



US010105664B2

(12) **United States Patent**
Hancock et al.

(10) **Patent No.:** **US 10,105,664 B2**
(45) **Date of Patent:** **Oct. 23, 2018**

(54) **RECIPROCATING TUBE-SHAKING MECHANISMS FOR PROCESSING A MATERIAL**

USPC 366/212, 215, 216, 217
See application file for complete search history.

(71) Applicant: **OMNI INTERNATIONAL, INC.**,
Kennesaw, GA (US)

(72) Inventors: **John Hancock**, Atlanta, GA (US);
Thomas Gray, Canton, GA (US);
Spencer Smith, Marietta, GA (US);
Voya Vidakovic, Marietta, GA (US);
Alan Vaughn, Dallas, TX (US)

(73) Assignee: **OMNI INTERNATIONAL, INC.**,
Kennesaw, GA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 199 days.

(21) Appl. No.: **14/926,731**

(22) Filed: **Oct. 29, 2015**

(65) **Prior Publication Data**

US 2016/0121278 A1 May 5, 2016

Related U.S. Application Data

(60) Provisional application No. 62/072,655, filed on Oct. 30, 2014.

(51) **Int. Cl.**
B01F 11/00 (2006.01)

(52) **U.S. Cl.**
CPC **B01F 11/0005** (2013.01); **B01F 11/0008** (2013.01); **B01F 11/0022** (2013.01); **B01F 2215/0037** (2013.01)

(58) **Field of Classification Search**
CPC B01F 11/0005; B01F 11/0008; B01F 11/0022; B01F 2215/0037

(56) **References Cited**

U.S. PATENT DOCUMENTS

67,095 A *	7/1867	Arnall	B01F 11/0005
				366/215
118,664 A *	8/1871	Yeager	B01F 11/0005
				366/215
140,280 A *	6/1873	Keeler	B01F 9/0025
				366/216
230,687 A *	8/1880	Baldwin	B01F 9/0025
				366/216
303,080 A *	8/1884	Wissenborn	B01F 11/0022
				366/212

(Continued)


Primary Examiner — Tony G Soohoo

(74) *Attorney, Agent, or Firm* — Gardner Groff
Greenwald & Villanueva, PC

(57) **ABSTRACT**

Agitation mechanisms for homogenization devices for processing sample materials in tubes that are secured by tube holders to the agitation mechanisms. Each agitation mechanism includes a first rotary member having a first fixed rotational axis, a second rotary member having a second fixed rotational axis, and a connecting member that extends between them, is rotationally mounted to them at third and fourth non-fixed rotational axes, and to which the tube holder is mounted, with the first and third rotational axes defining a first offset, and with the second and fourth rotational axes defining a second offset. When the first rotary member is driven through rotation, the sample in the tube in the tube holder on the connecting member is driven through a nonlinearly reciprocating motion profile to produce a grinding shear action to better homogenize the samples. Other disclosed embodiments produce linearly reciprocating motion profiles.

11 Claims, 18 Drawing Sheets

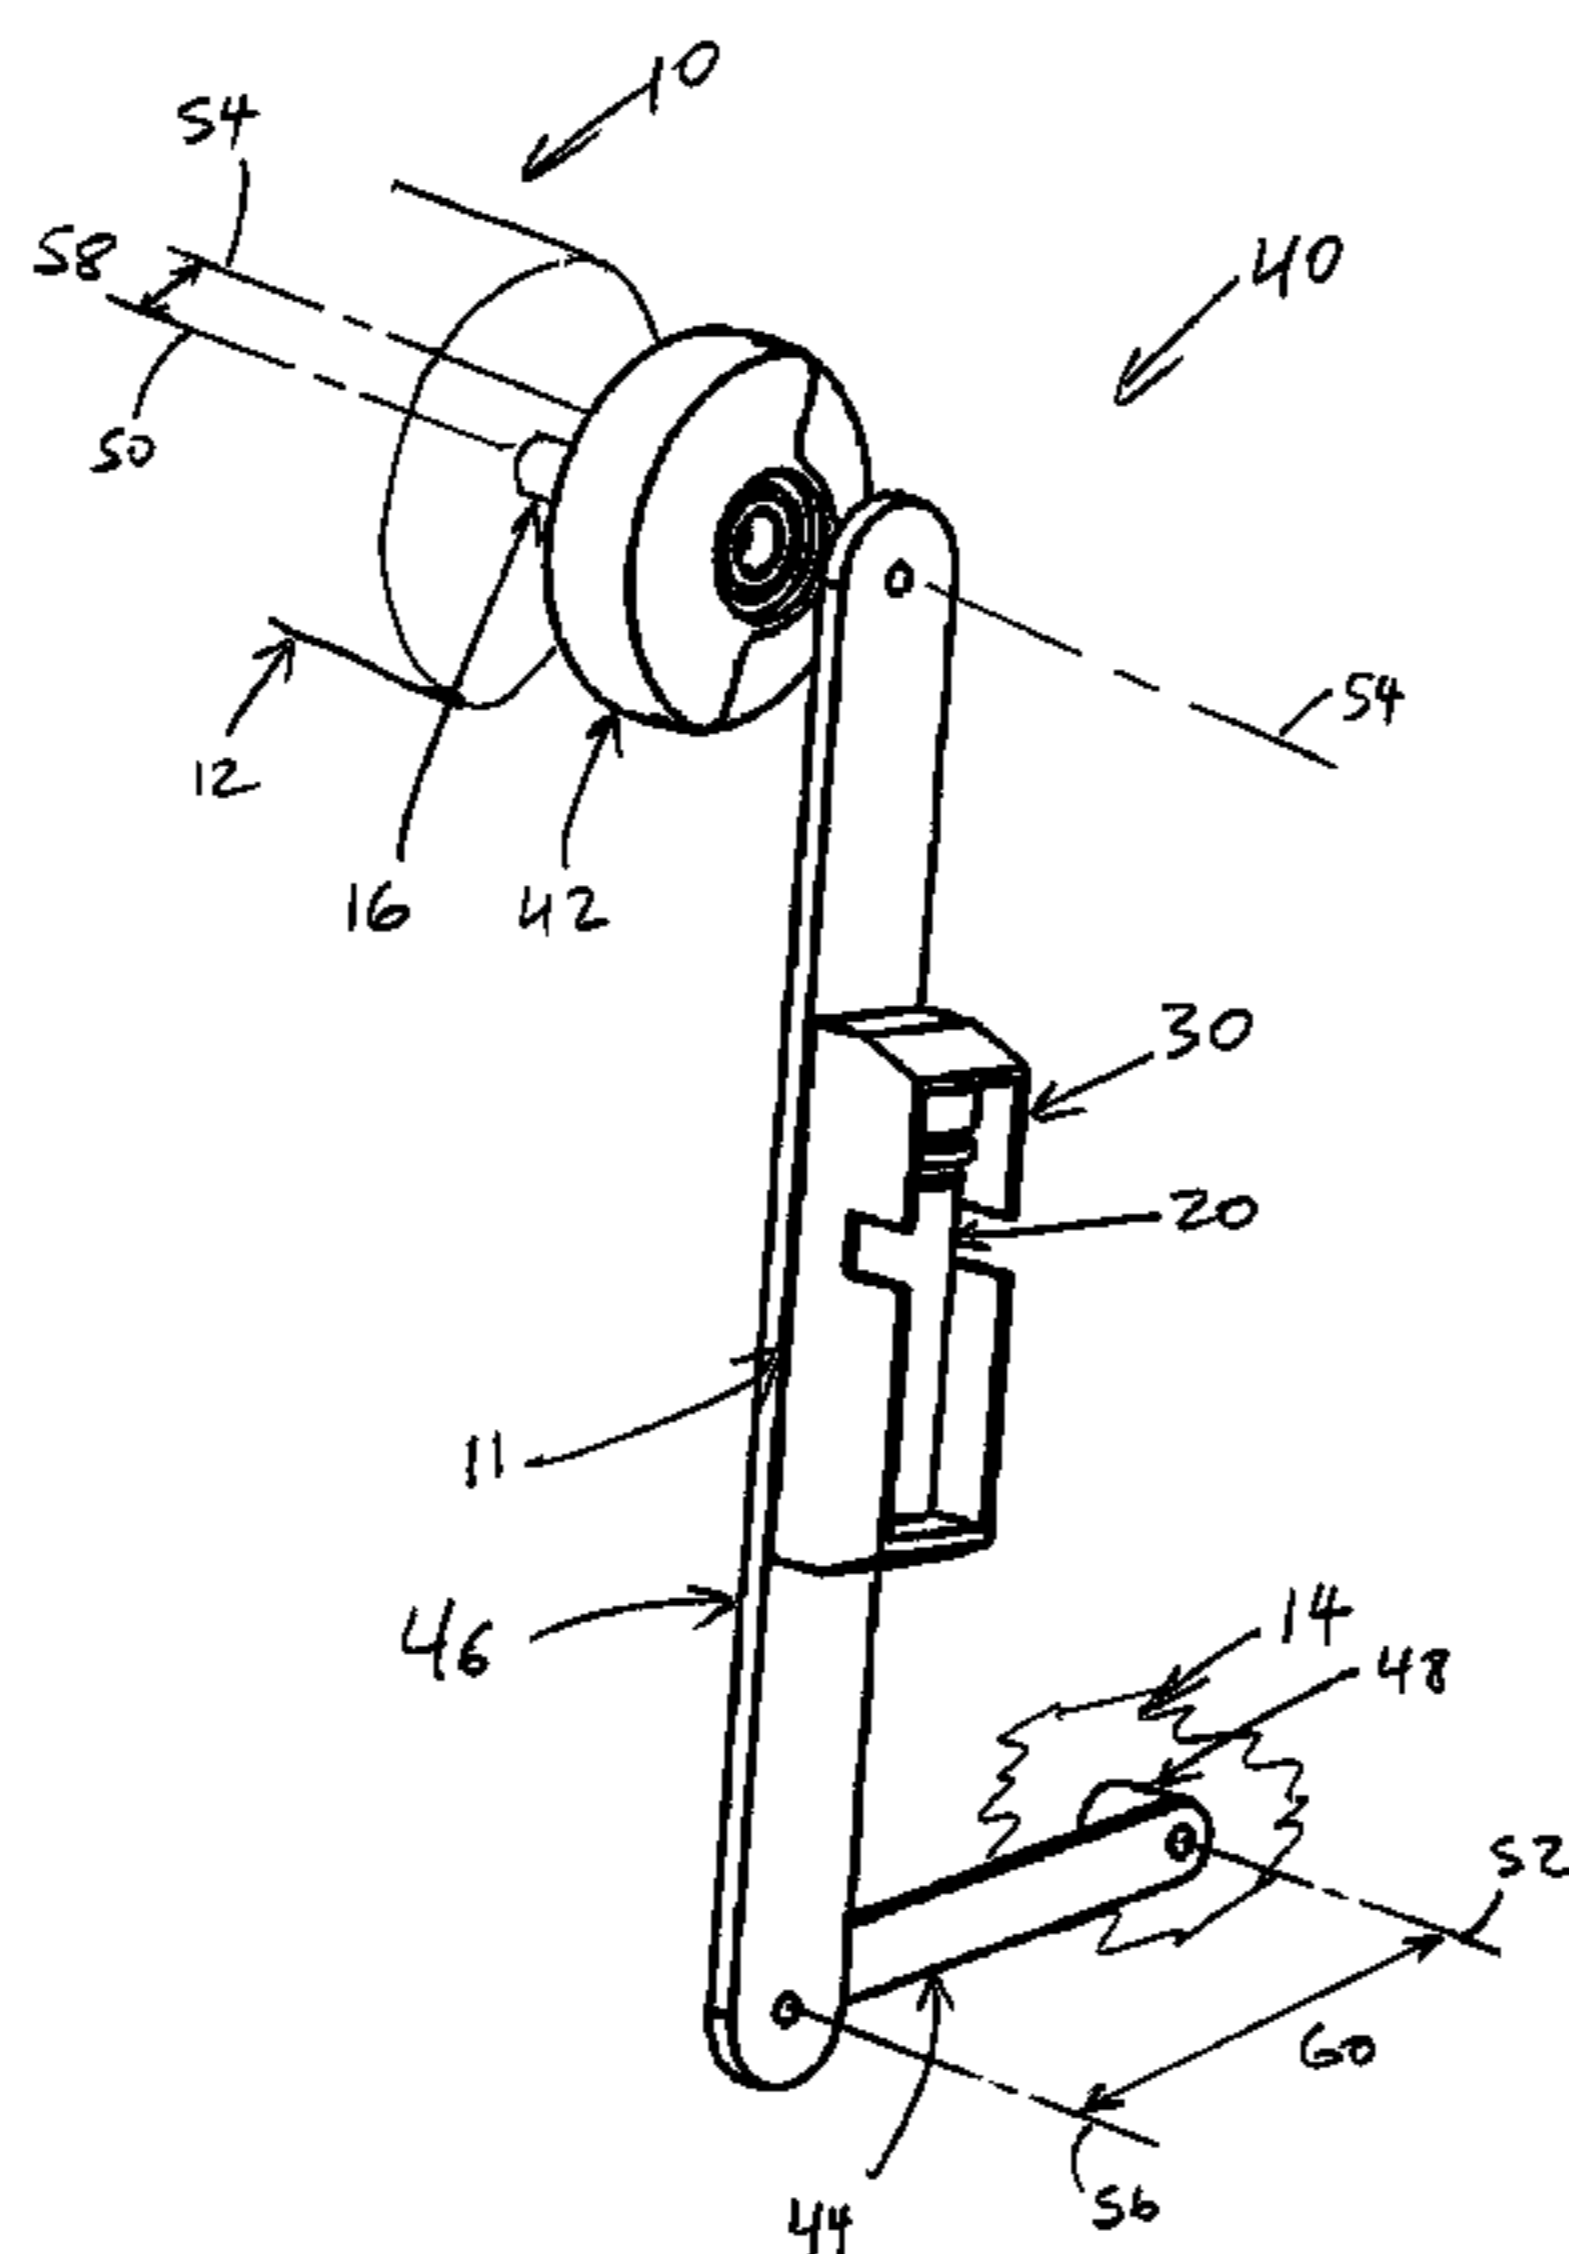


(56)

References Cited

U.S. PATENT DOCUMENTS

390,974 A *	10/1888	Jennings	B01F 11/0022	366/212	1,704,010 A *	3/1929	Manon	B01F 11/0022	366/212
391,150 A *	10/1888	Jennings	B01F 11/0022	366/212	2,146,860 A *	2/1939	Shaw	A47J 43/042	366/212
392,865 A *	11/1888	Kanable	B01F 11/0008	366/110	2,345,130 A *	3/1944	Latham	B01F 11/0022	366/215
639,404 A *	12/1899	Kolls	B01F 11/0022	366/212	2,673,722 A *	3/1954	Griffin	B01F 11/0022	366/212
791,664 A *	6/1905	Wilson	B01F 11/0022	366/209	3,198,502 A *	8/1965	Thompson	B01F 11/0022	210/388
985,040 A *	2/1911	Lillienthal	B01F 11/0022	366/212	3,437,317 A *	4/1969	Micin	A47J 43/042	366/211
1,015,383 A *	1/1912	Dyer	B01F 11/0022	366/212	5,608,693 A *	3/1997	Richards	B01F 11/0005	366/114
1,242,218 A *	10/1917	McCann	B01F 11/0022	366/212	5,697,701 A *	12/1997	Forrest	B01F 11/0031	366/110
1,329,843 A *	2/1920	Meguiar	B01F 11/0022	366/212	8,889,406 B2 *	11/2014	van der Heiden ..	B01F 11/0025	366/211	
1,365,963 A *	1/1921	Brown	A01J 15/04	366/210	2012/0263010 A1 *	10/2012	Boquet	B01F 11/0008	366/110
RE15,677 E *	8/1923	Brown et al.	A01J 15/04	366/215	2013/0003487 A1 *	1/2013	Ballard	B01F 11/0008	366/110
1,486,266 A *	3/1924	Rosenblatt	B01F 11/0022	366/212	2014/0072474 A1	3/2014	Kido et al.			
1,527,227 A *	2/1925	Sanders	A47J 43/042	366/212	2014/0126321 A1 *	5/2014	Eisen	B01F 15/00409	366/213
						2014/0212336 A1	7/2014	Kido et al.			
						2016/0121278 A1 *	5/2016	Hancock	B01F 11/0005	366/215

* cited by examiner

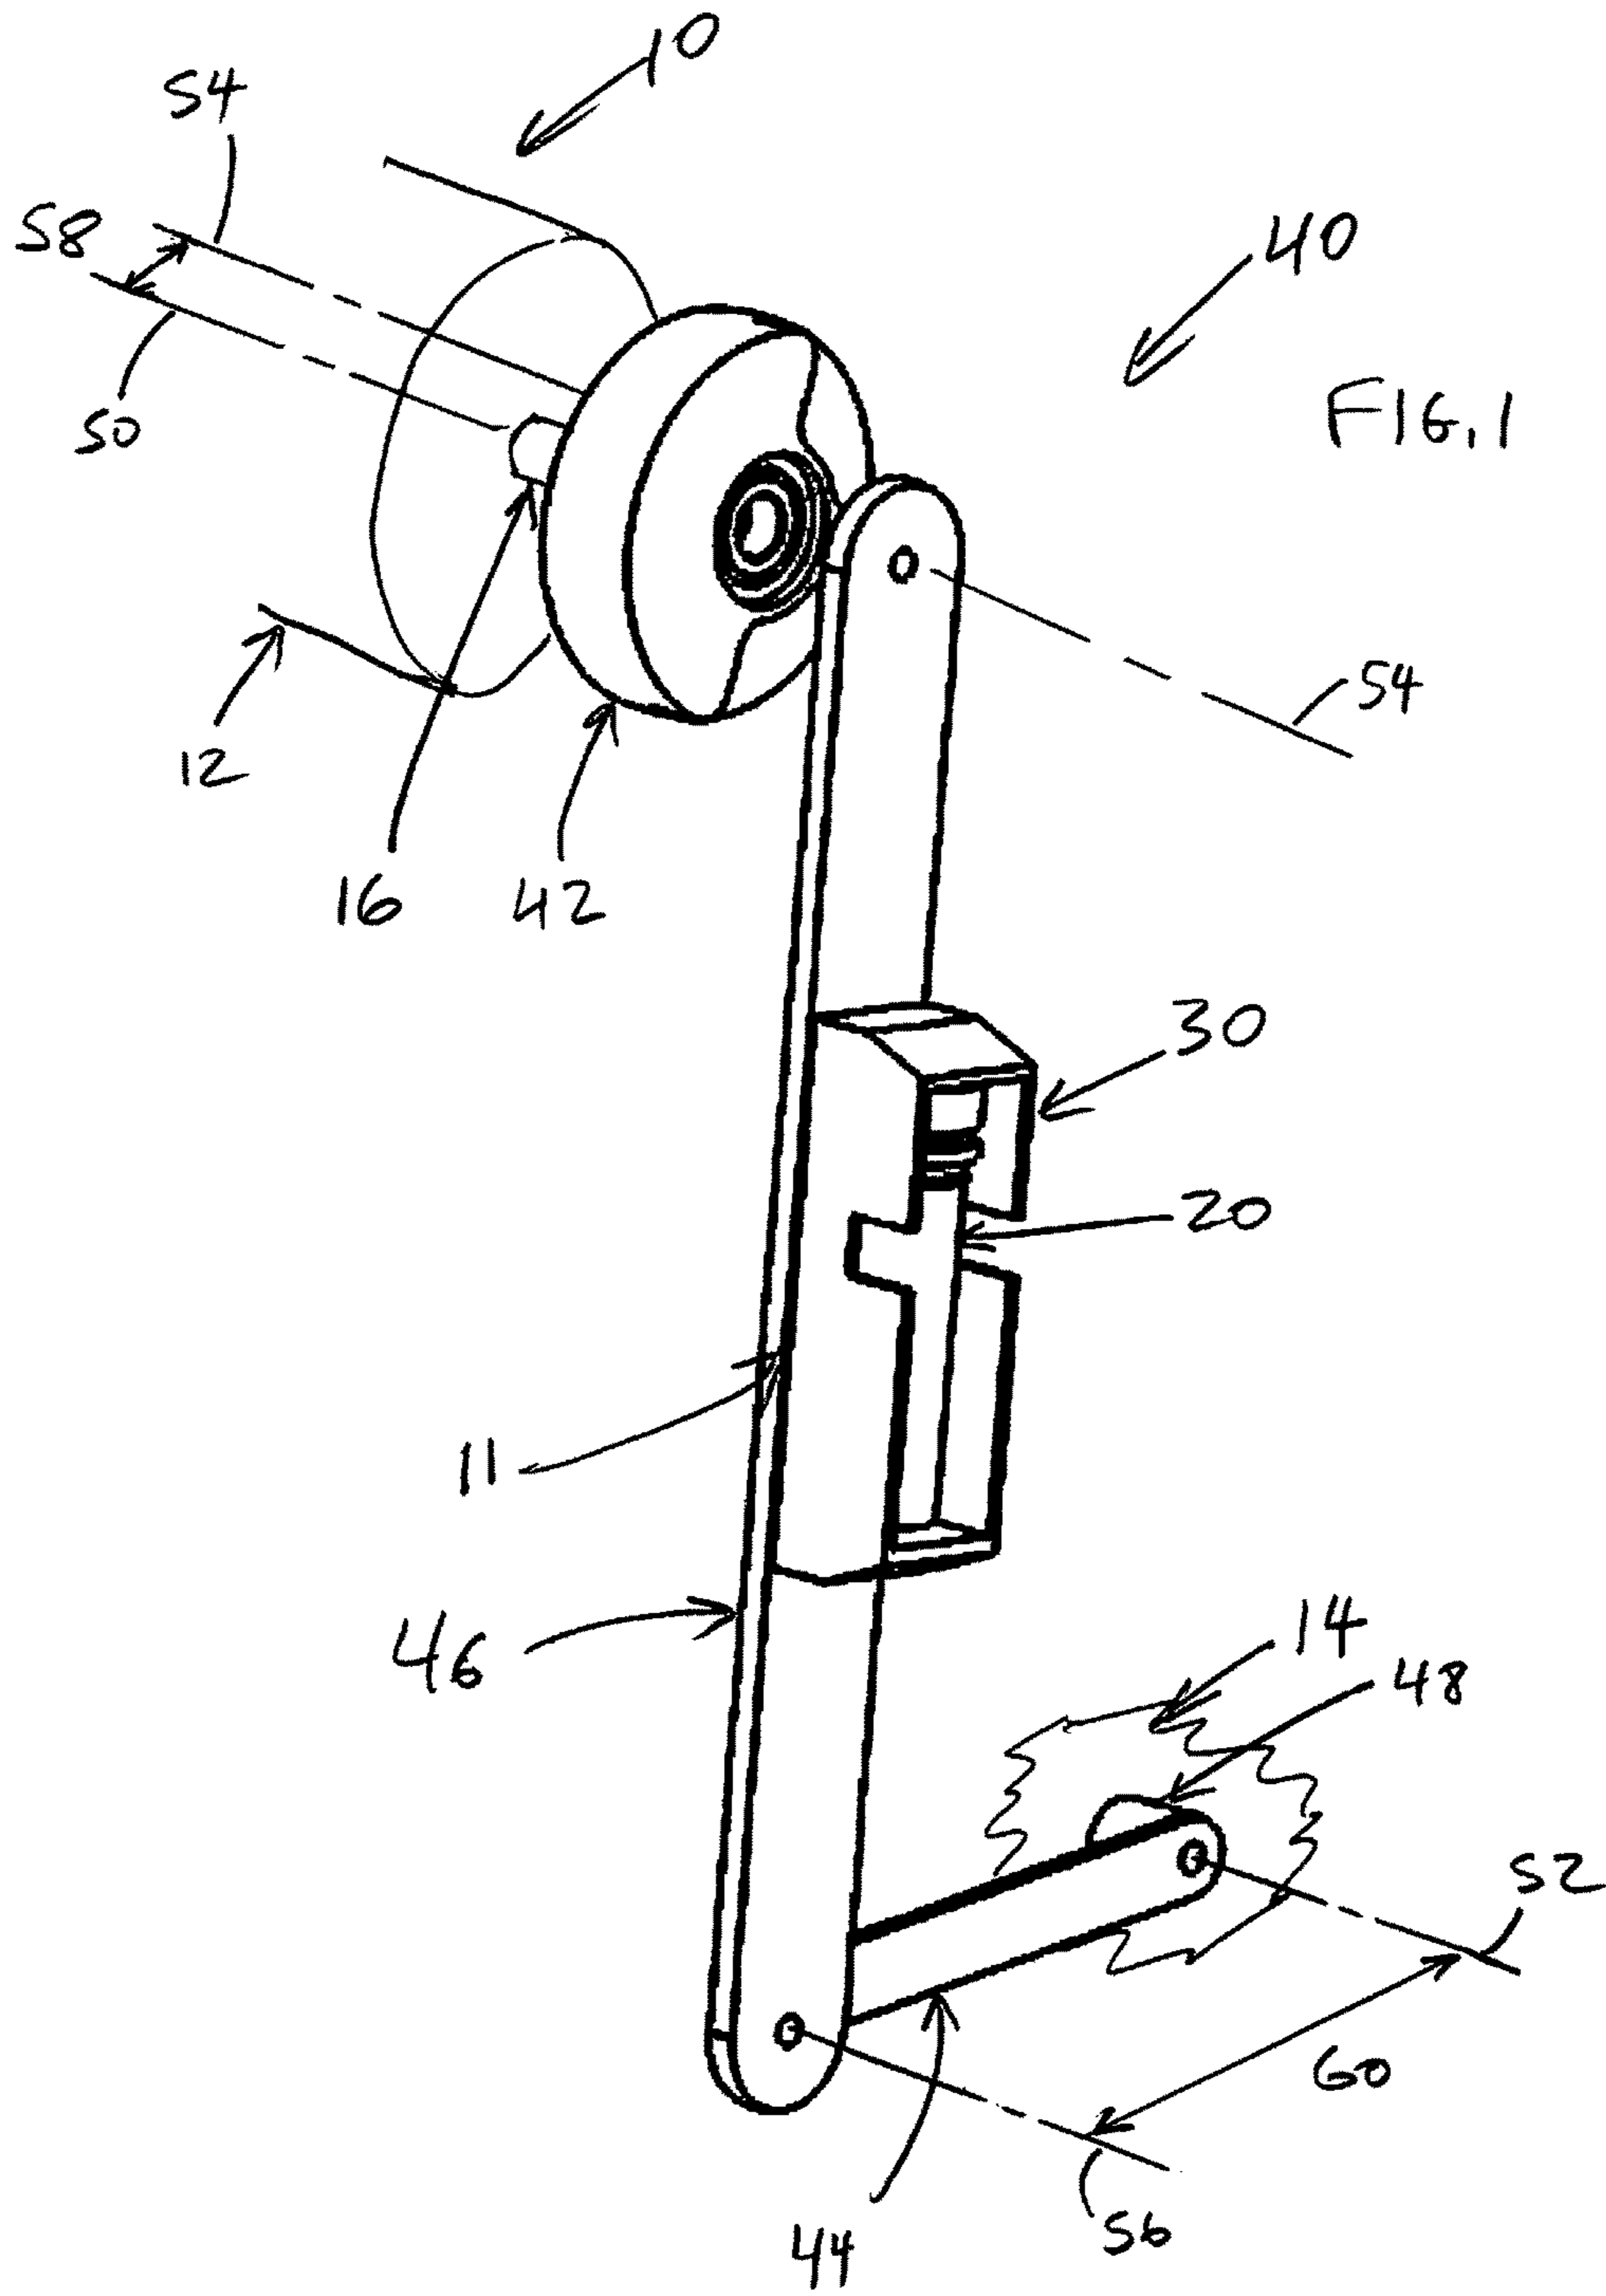

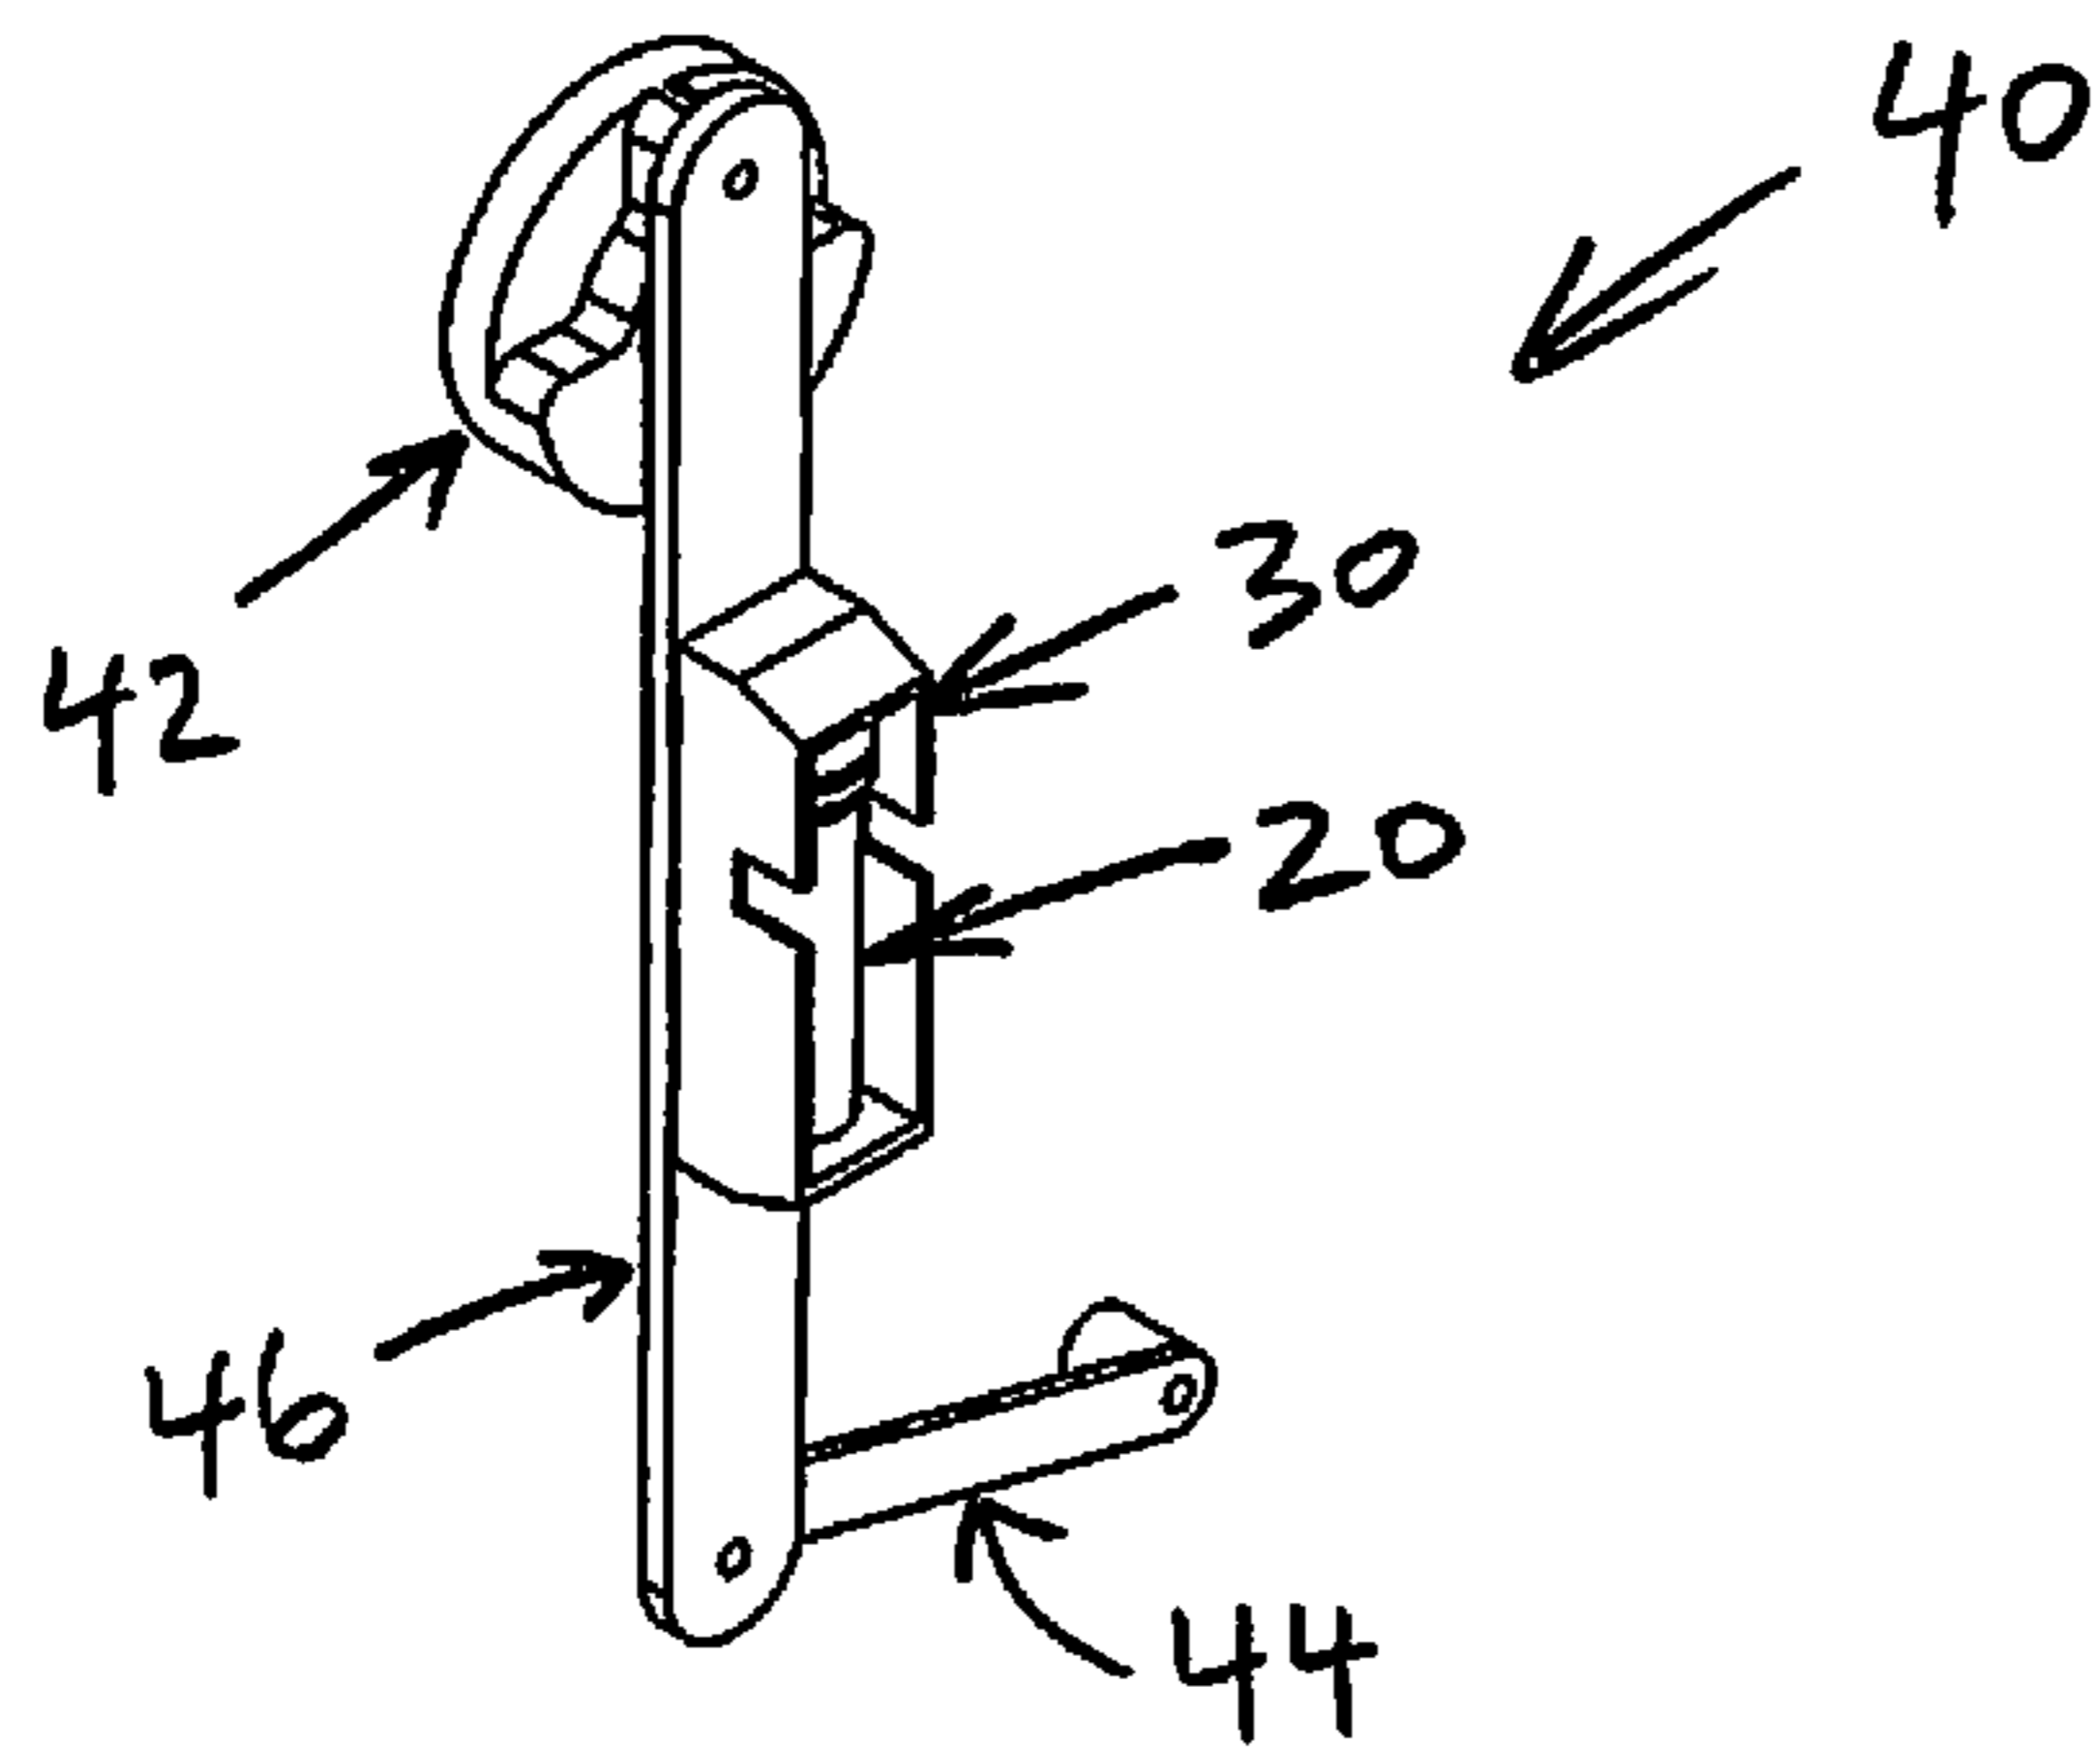


FIG. 2



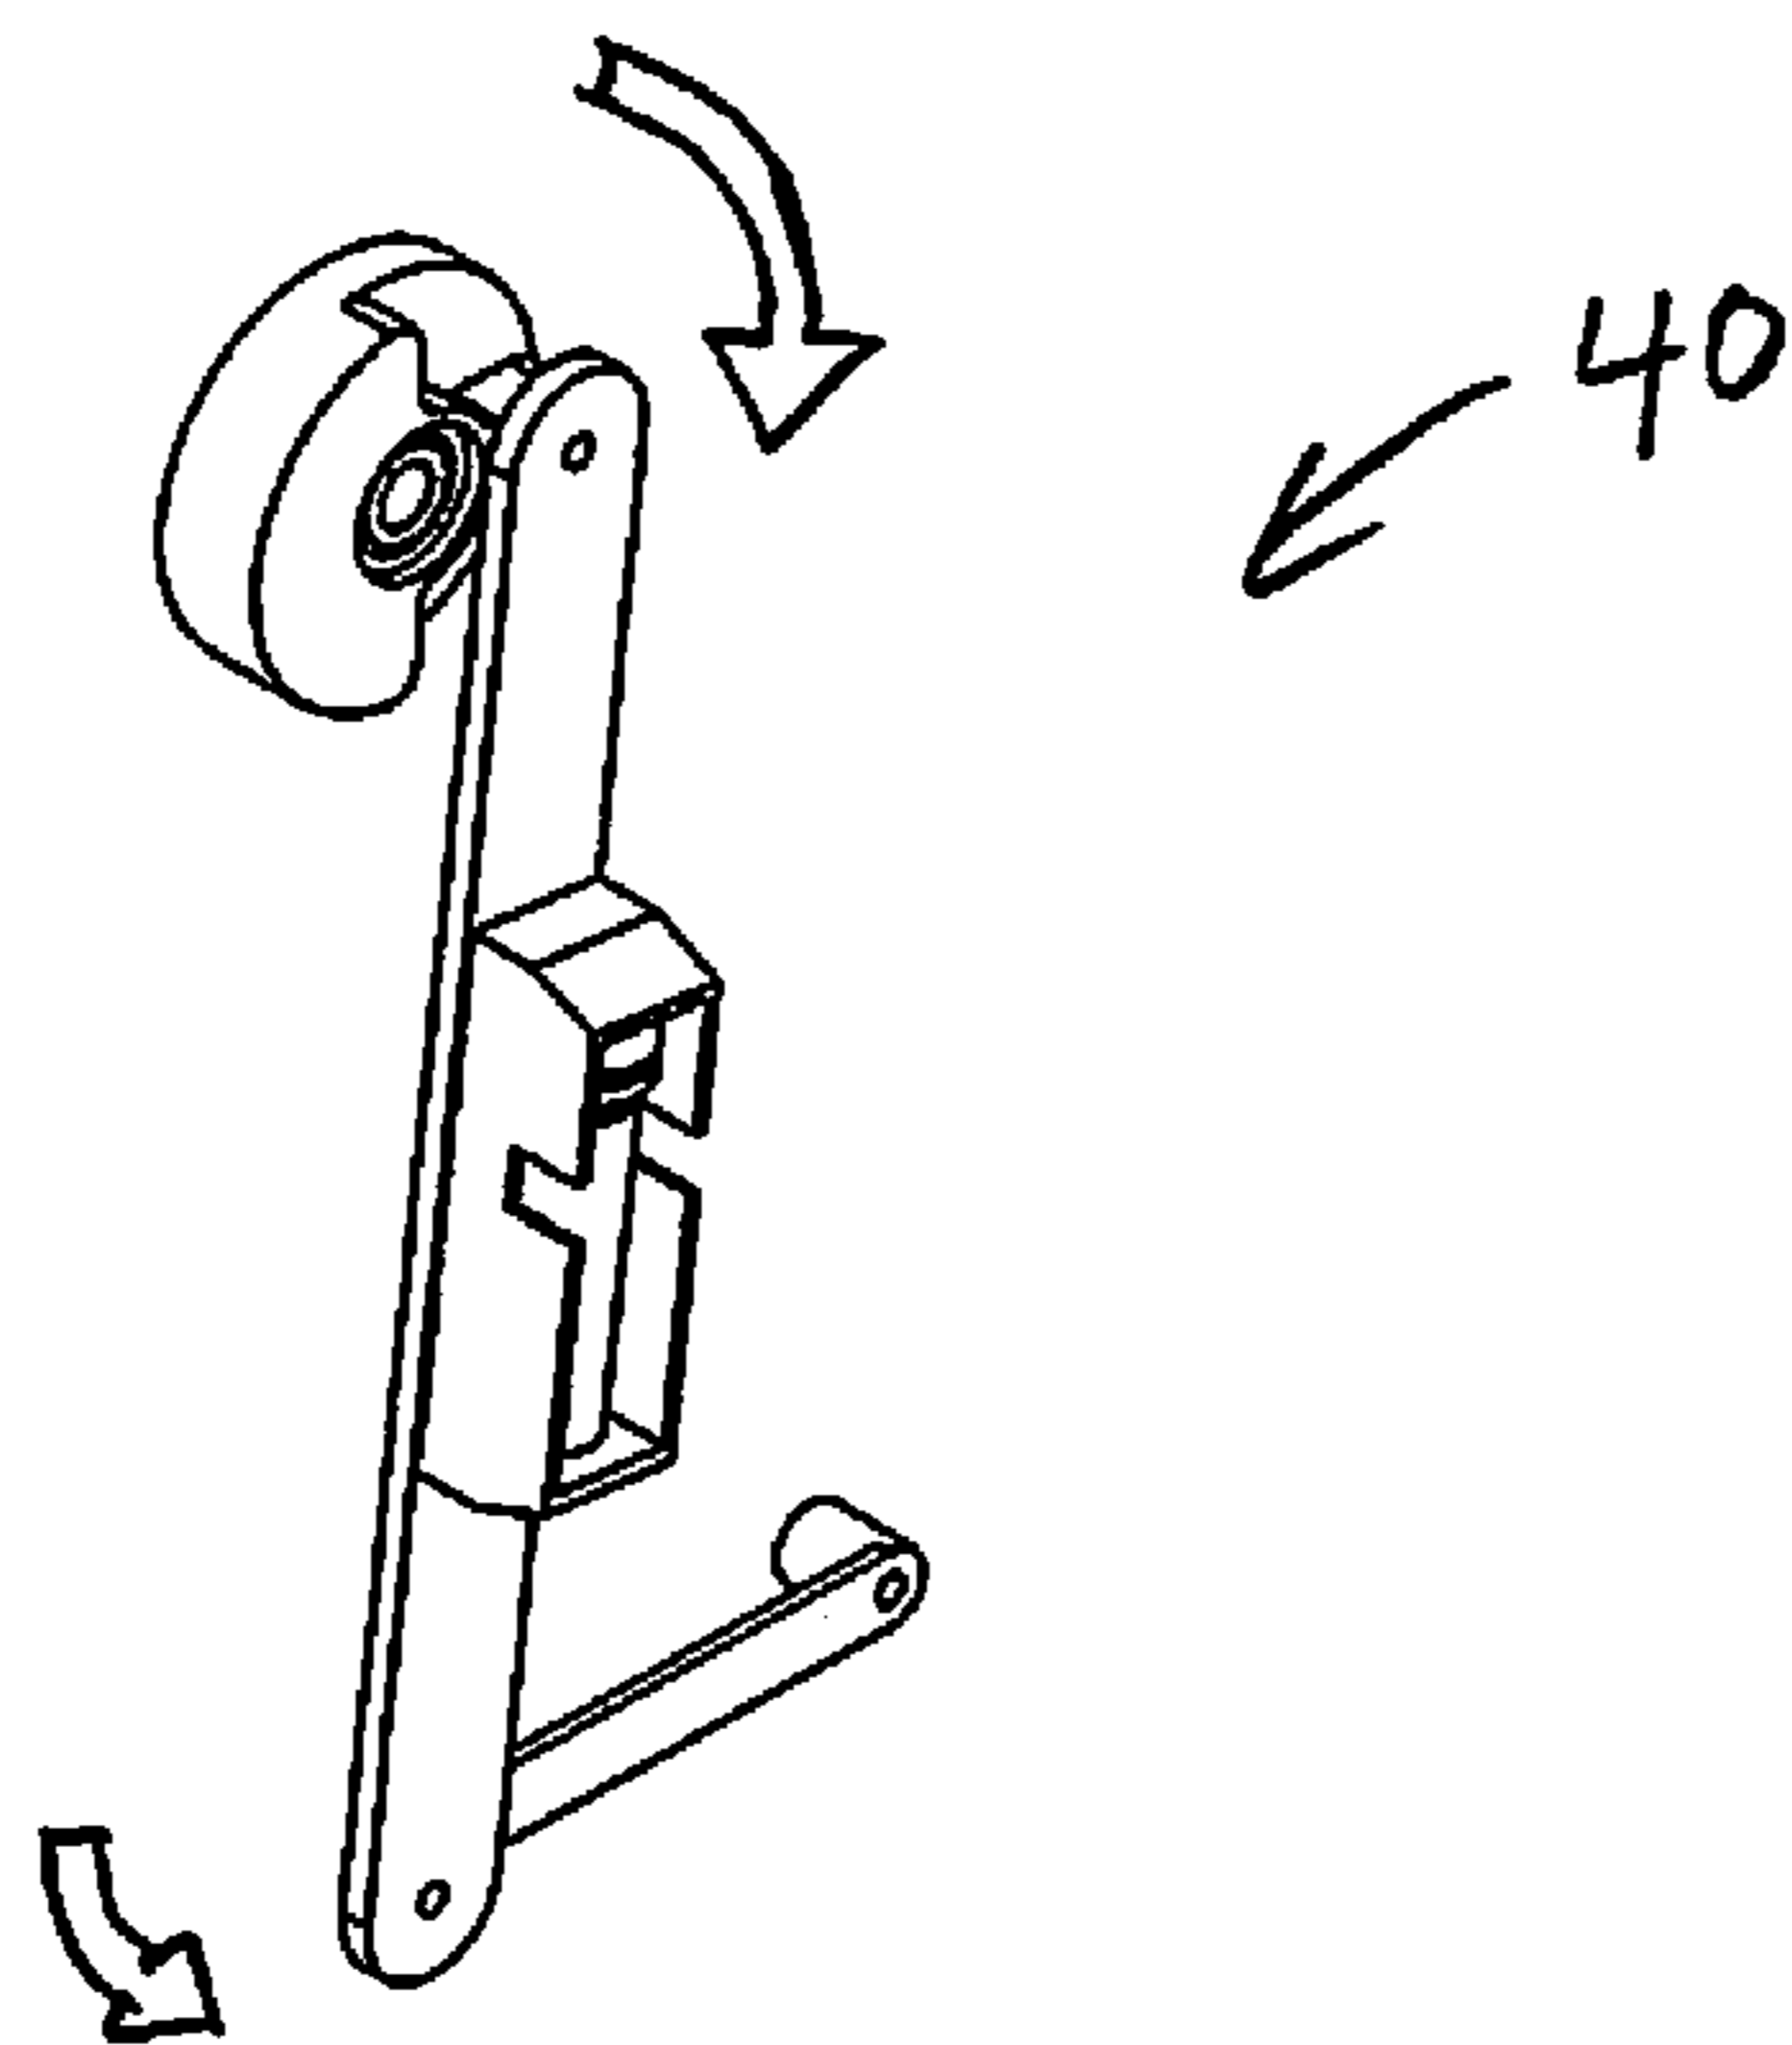


FIG. 3

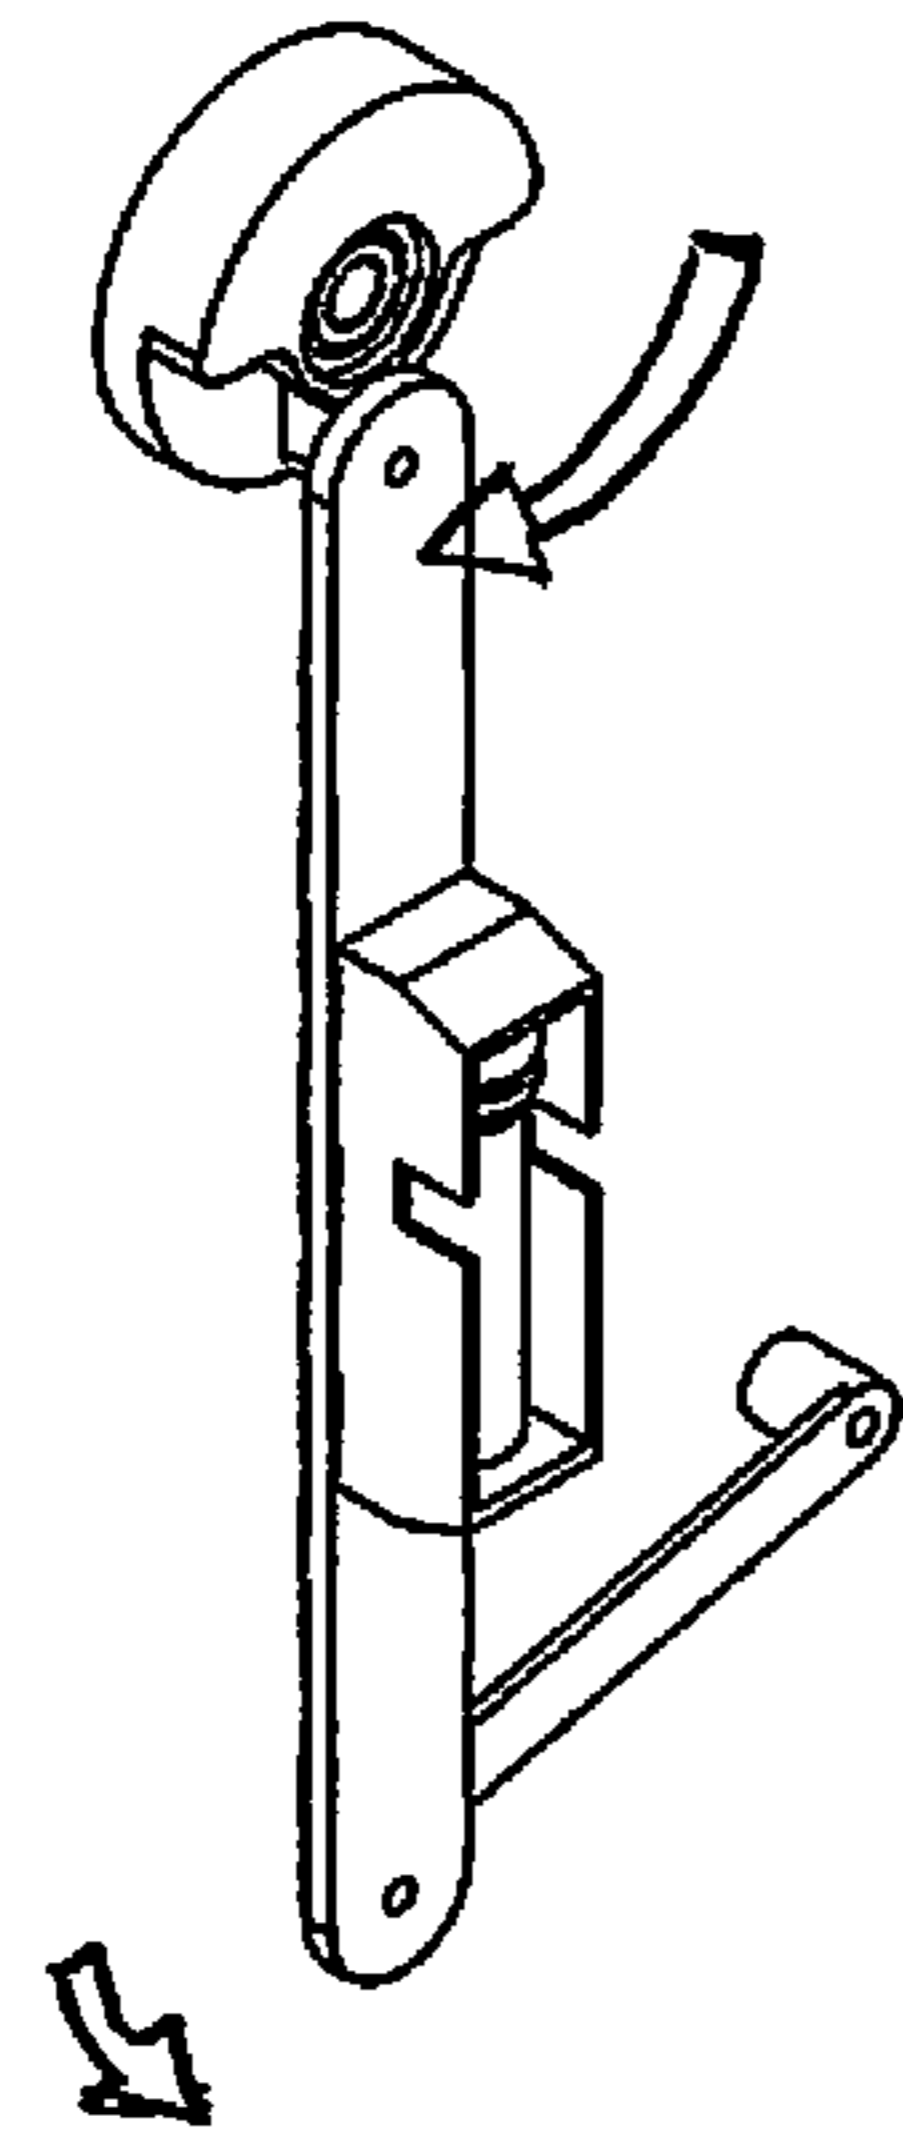

40

FIG. 4

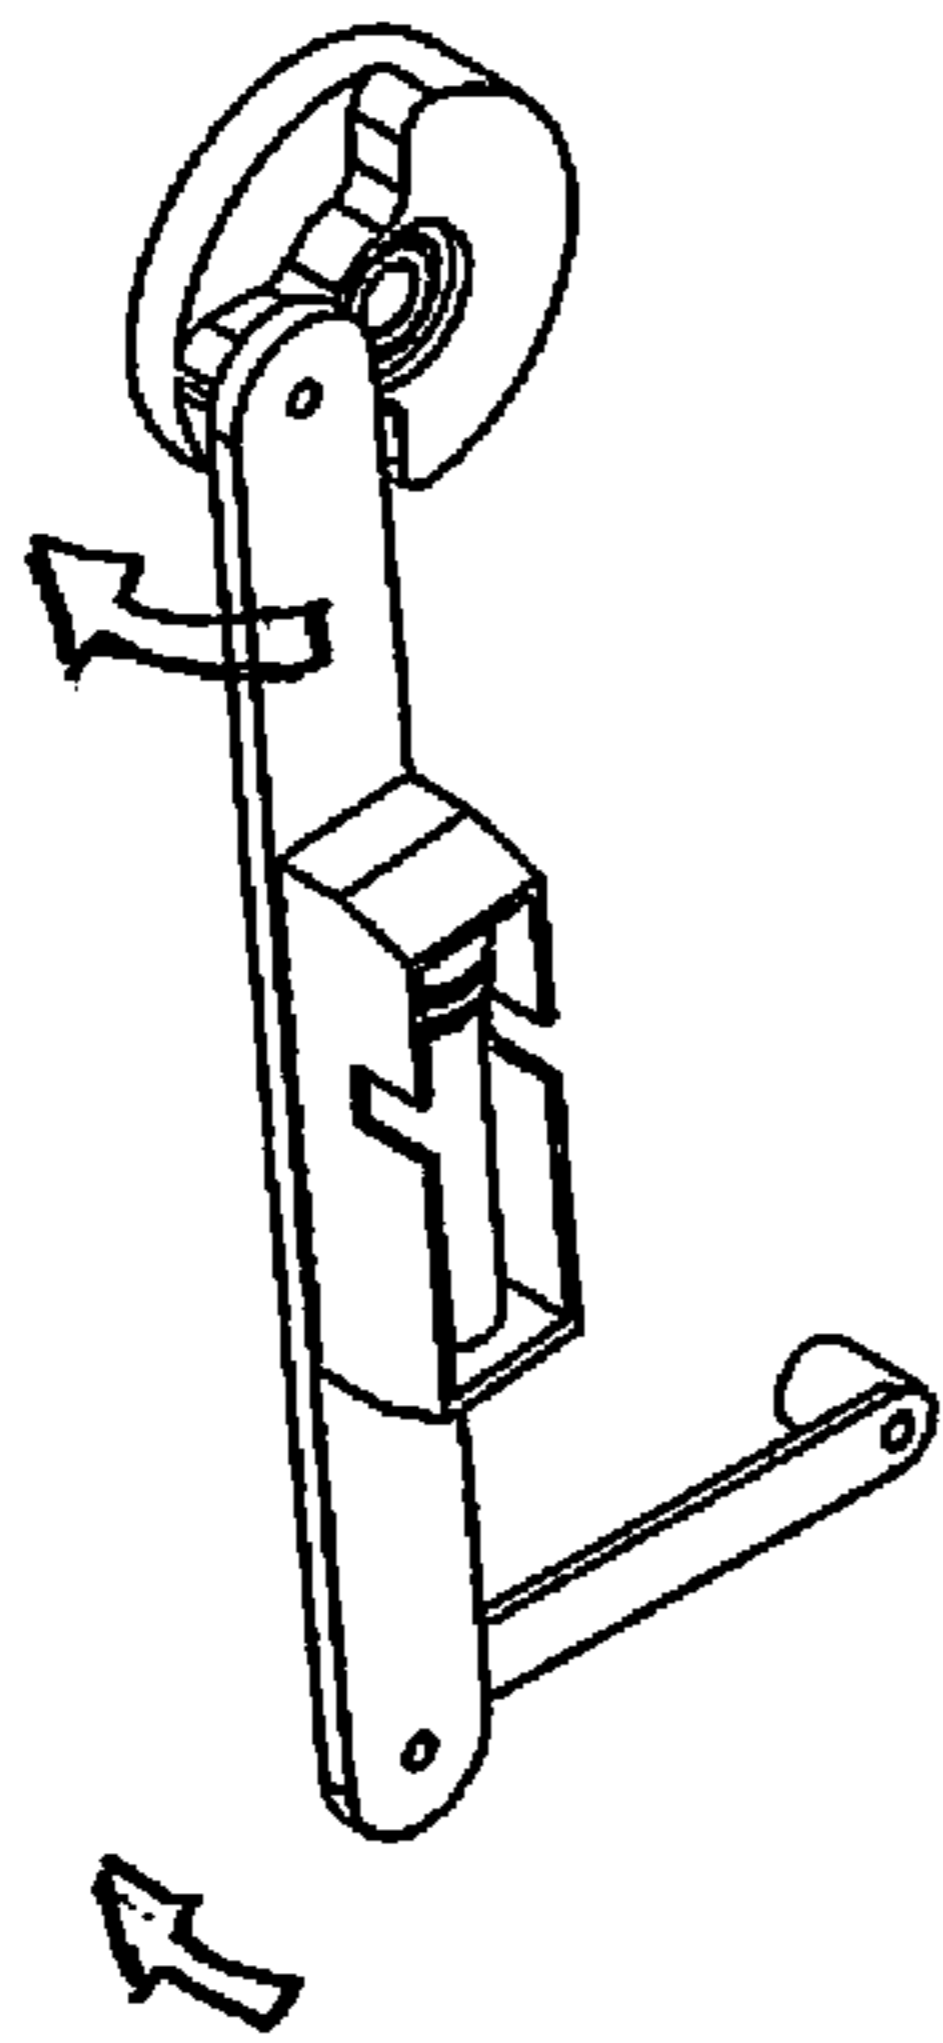

40

FIG. 5



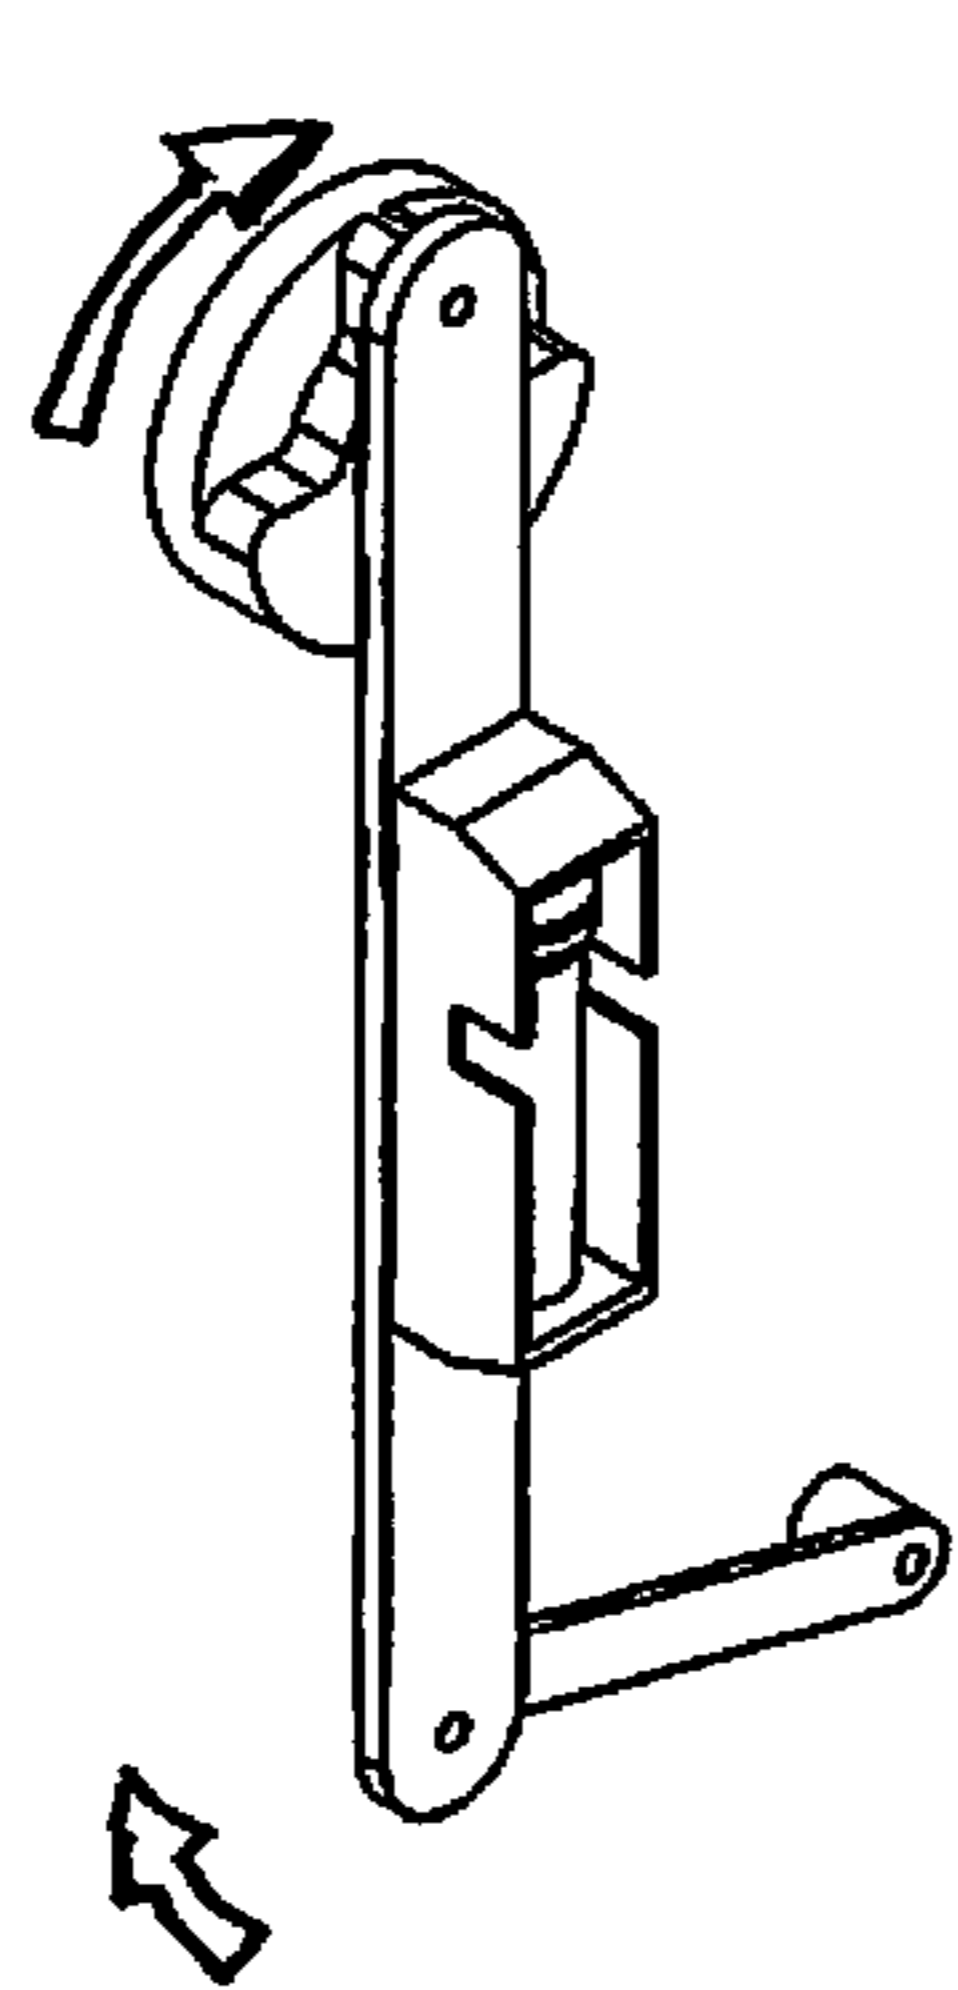


FIG. 6

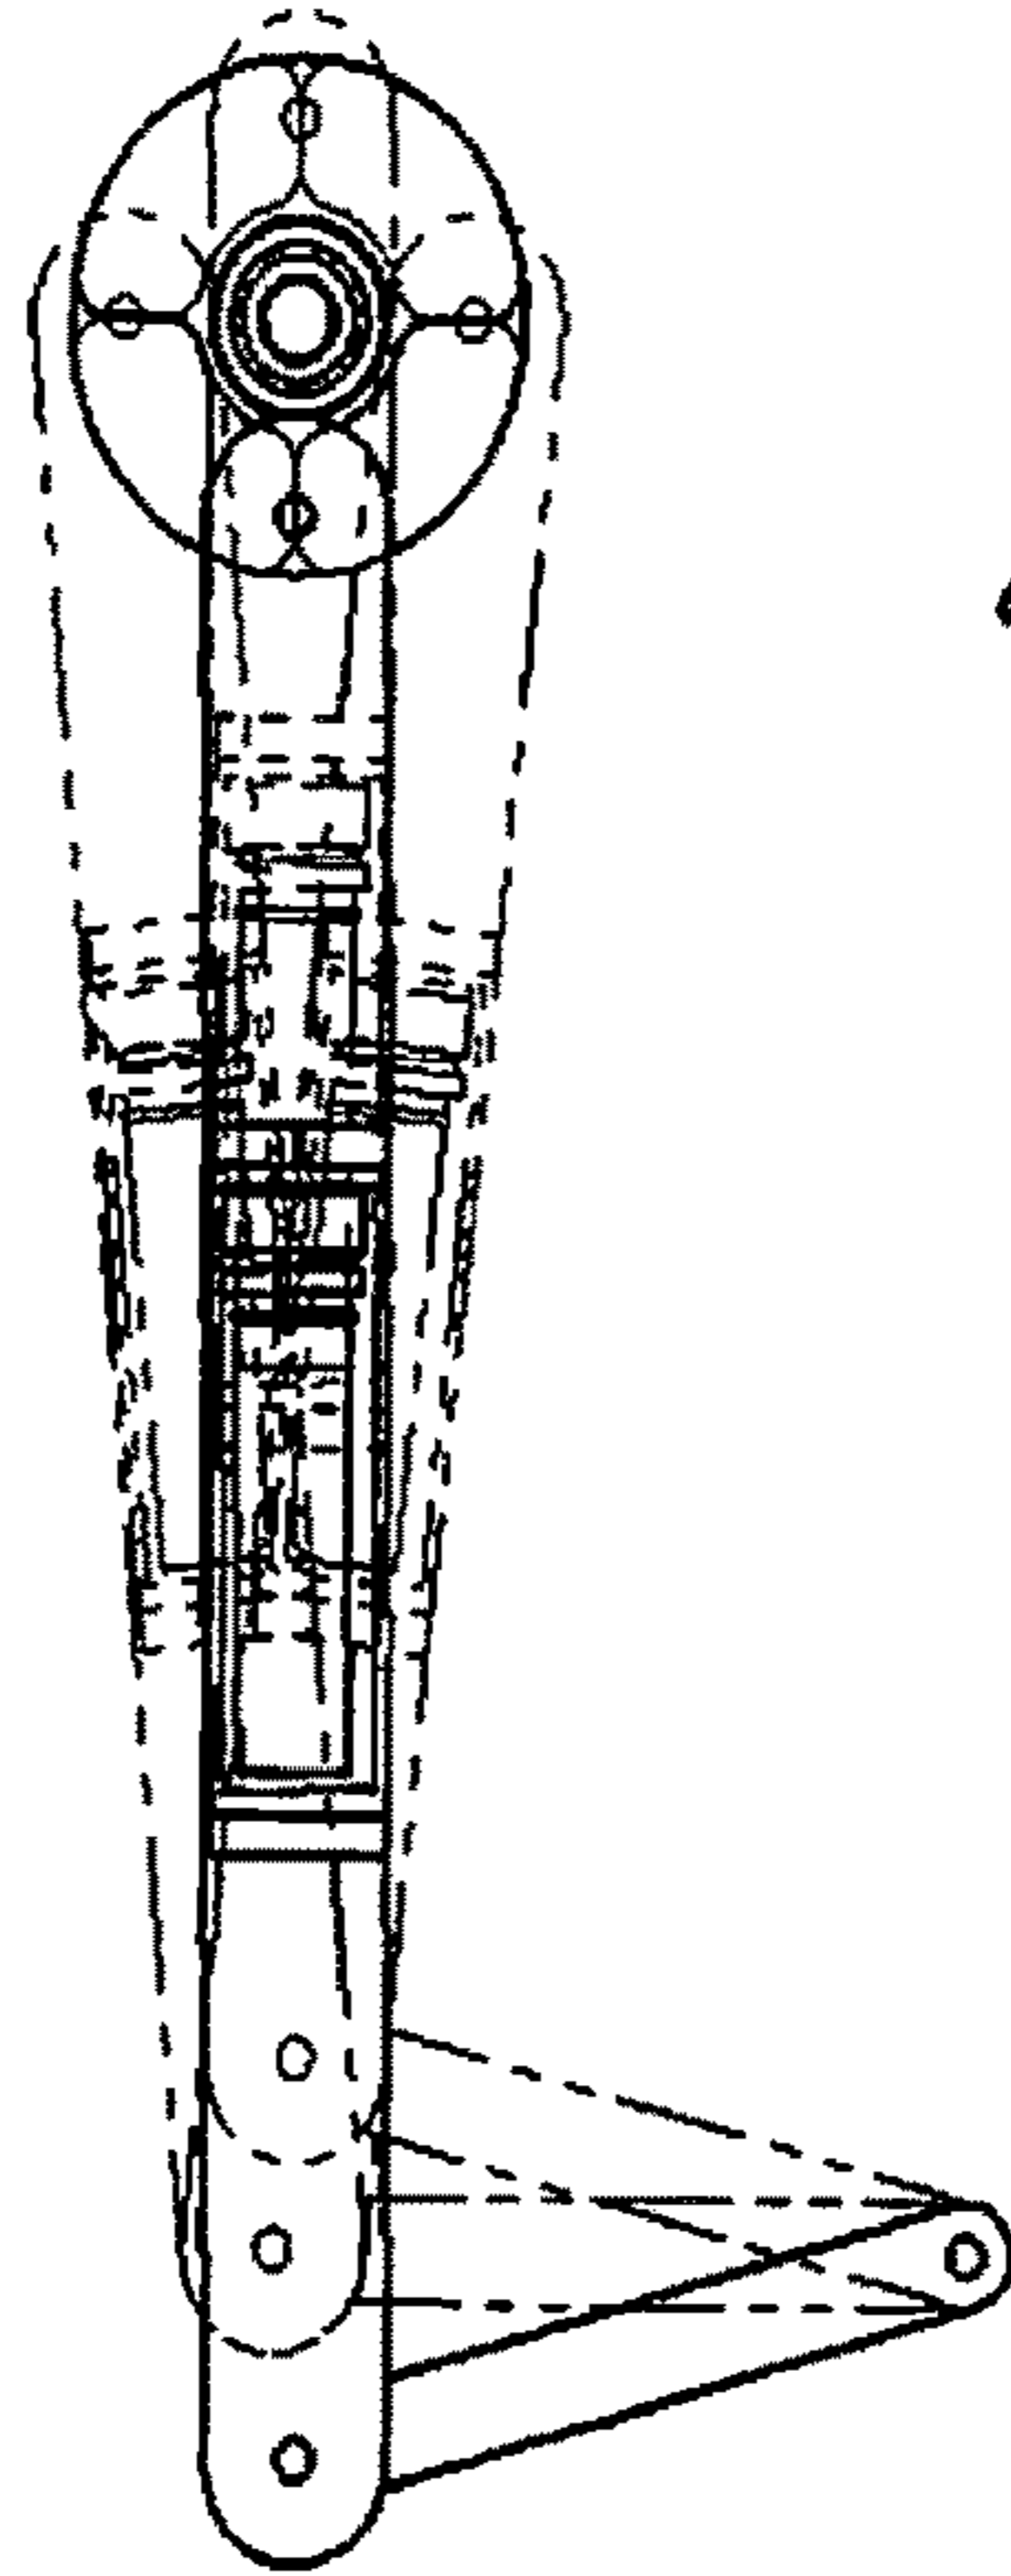


← 40

FIG. 7

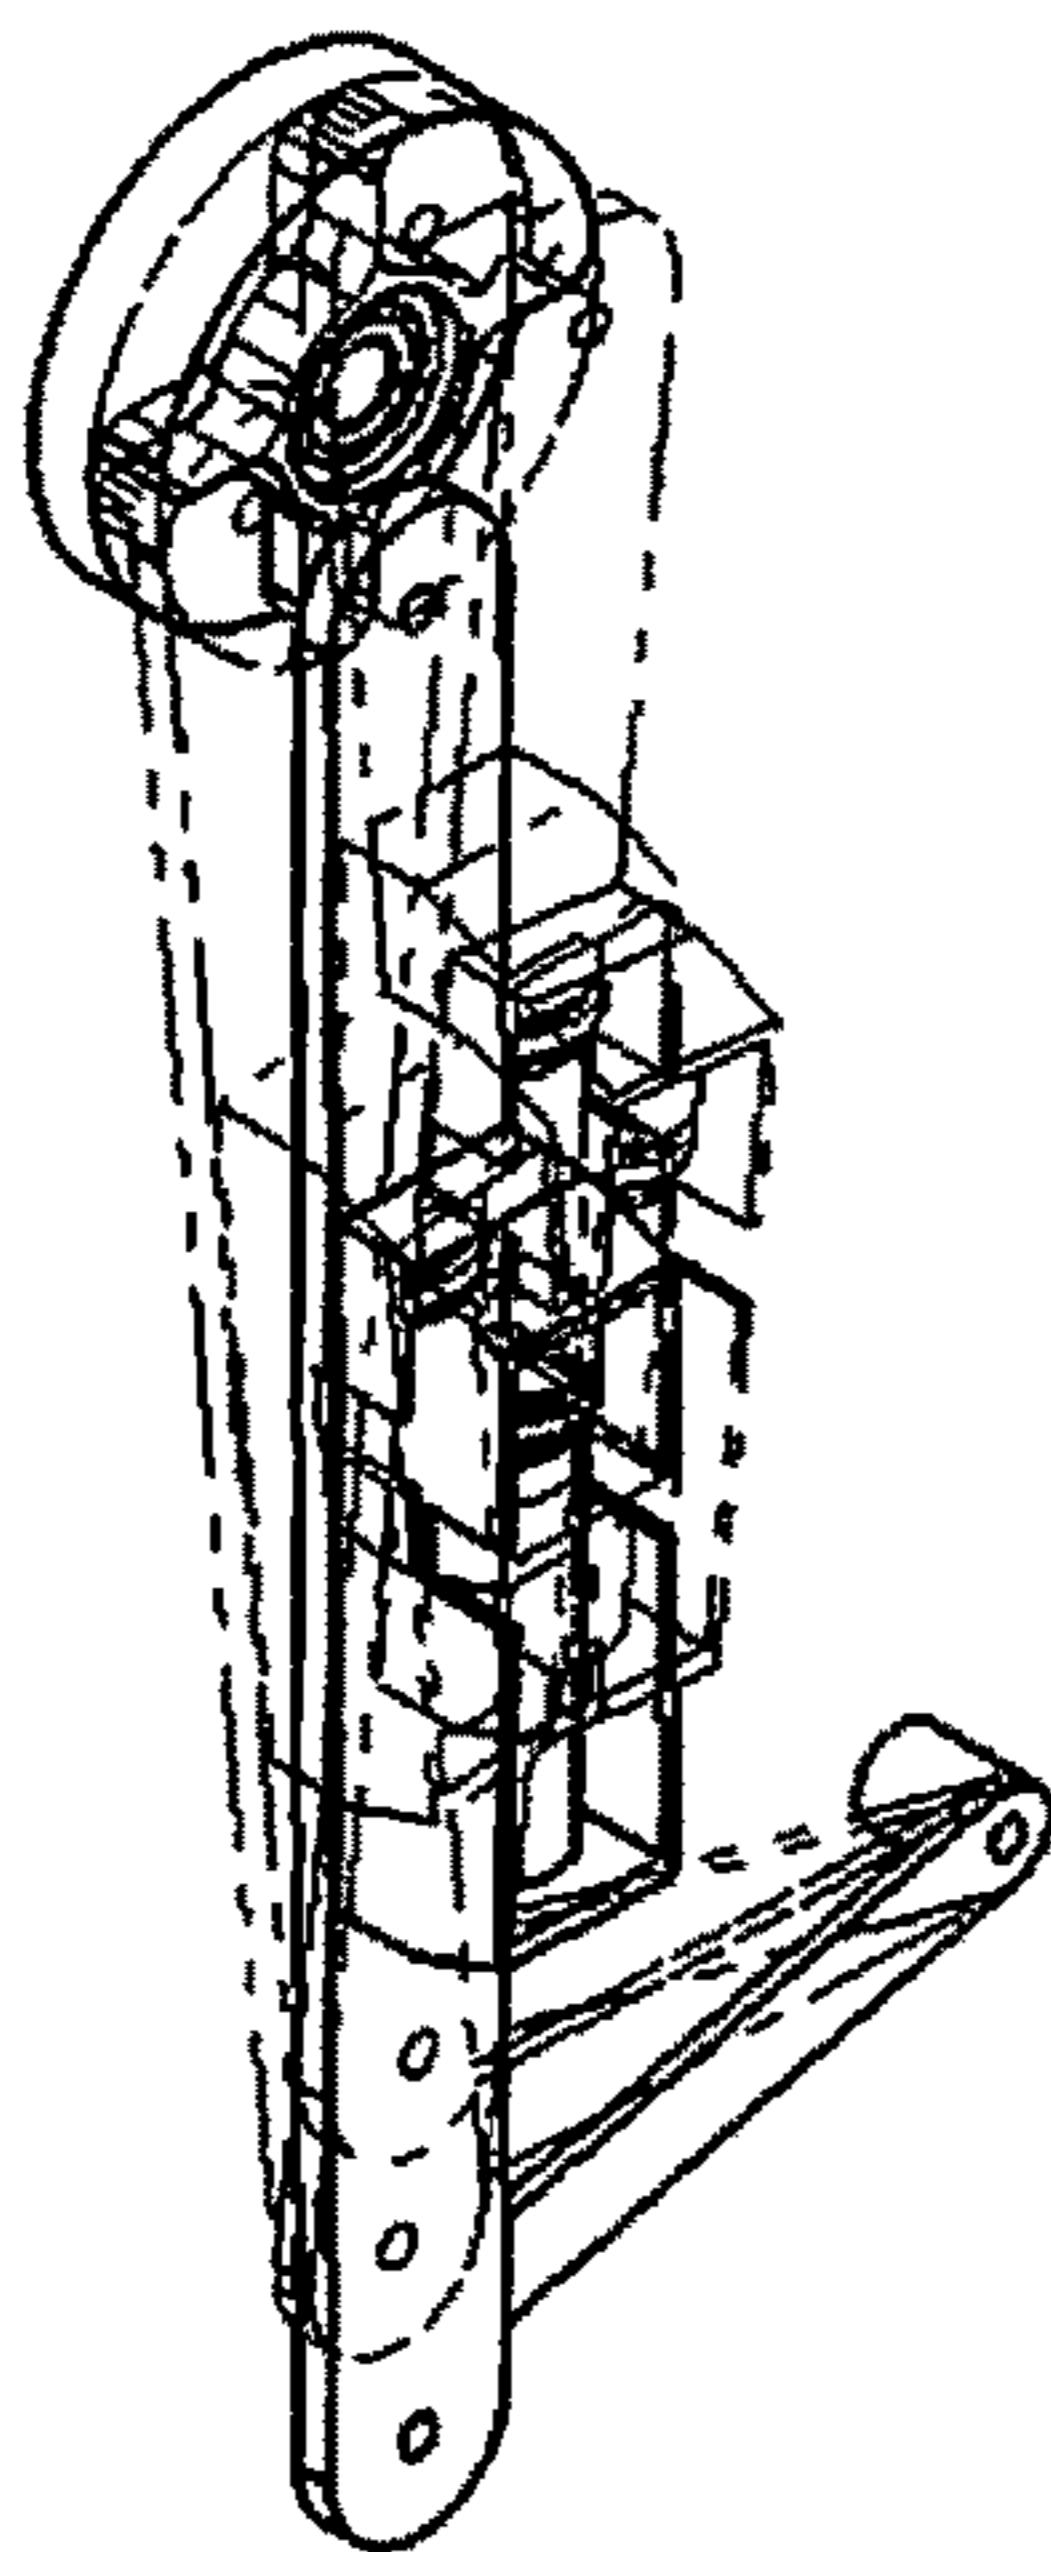

← 40

FIG. 8

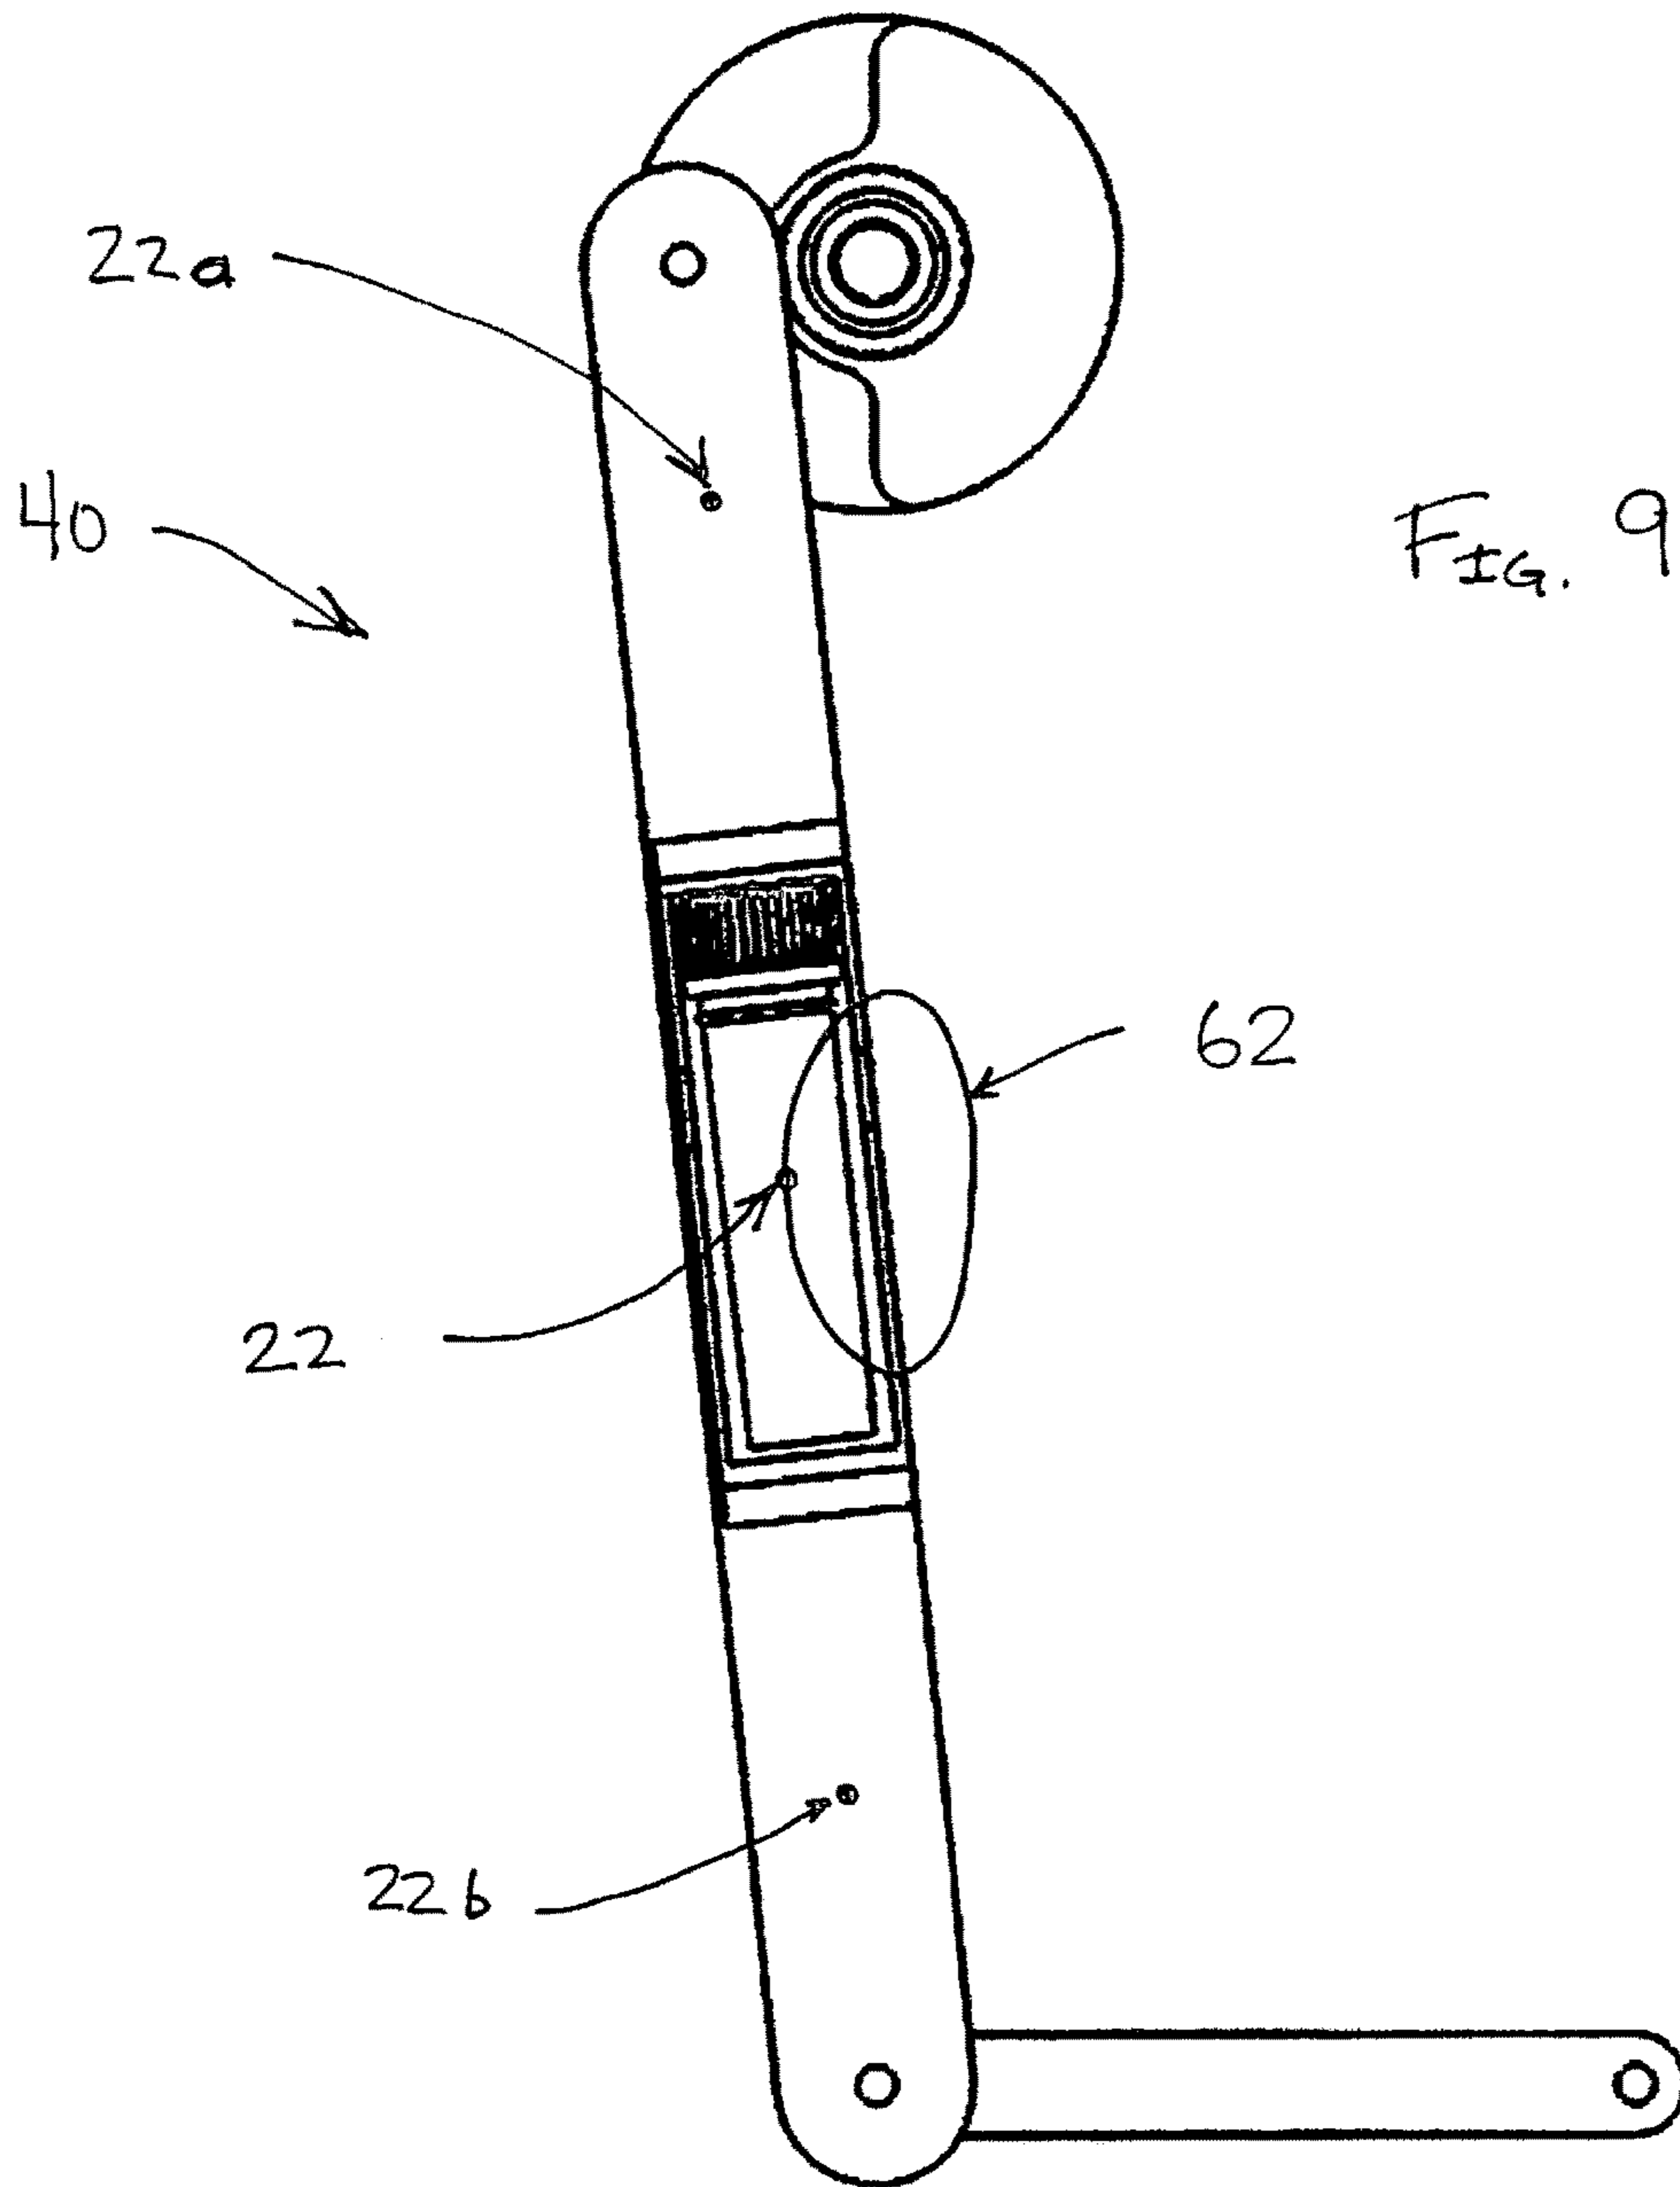



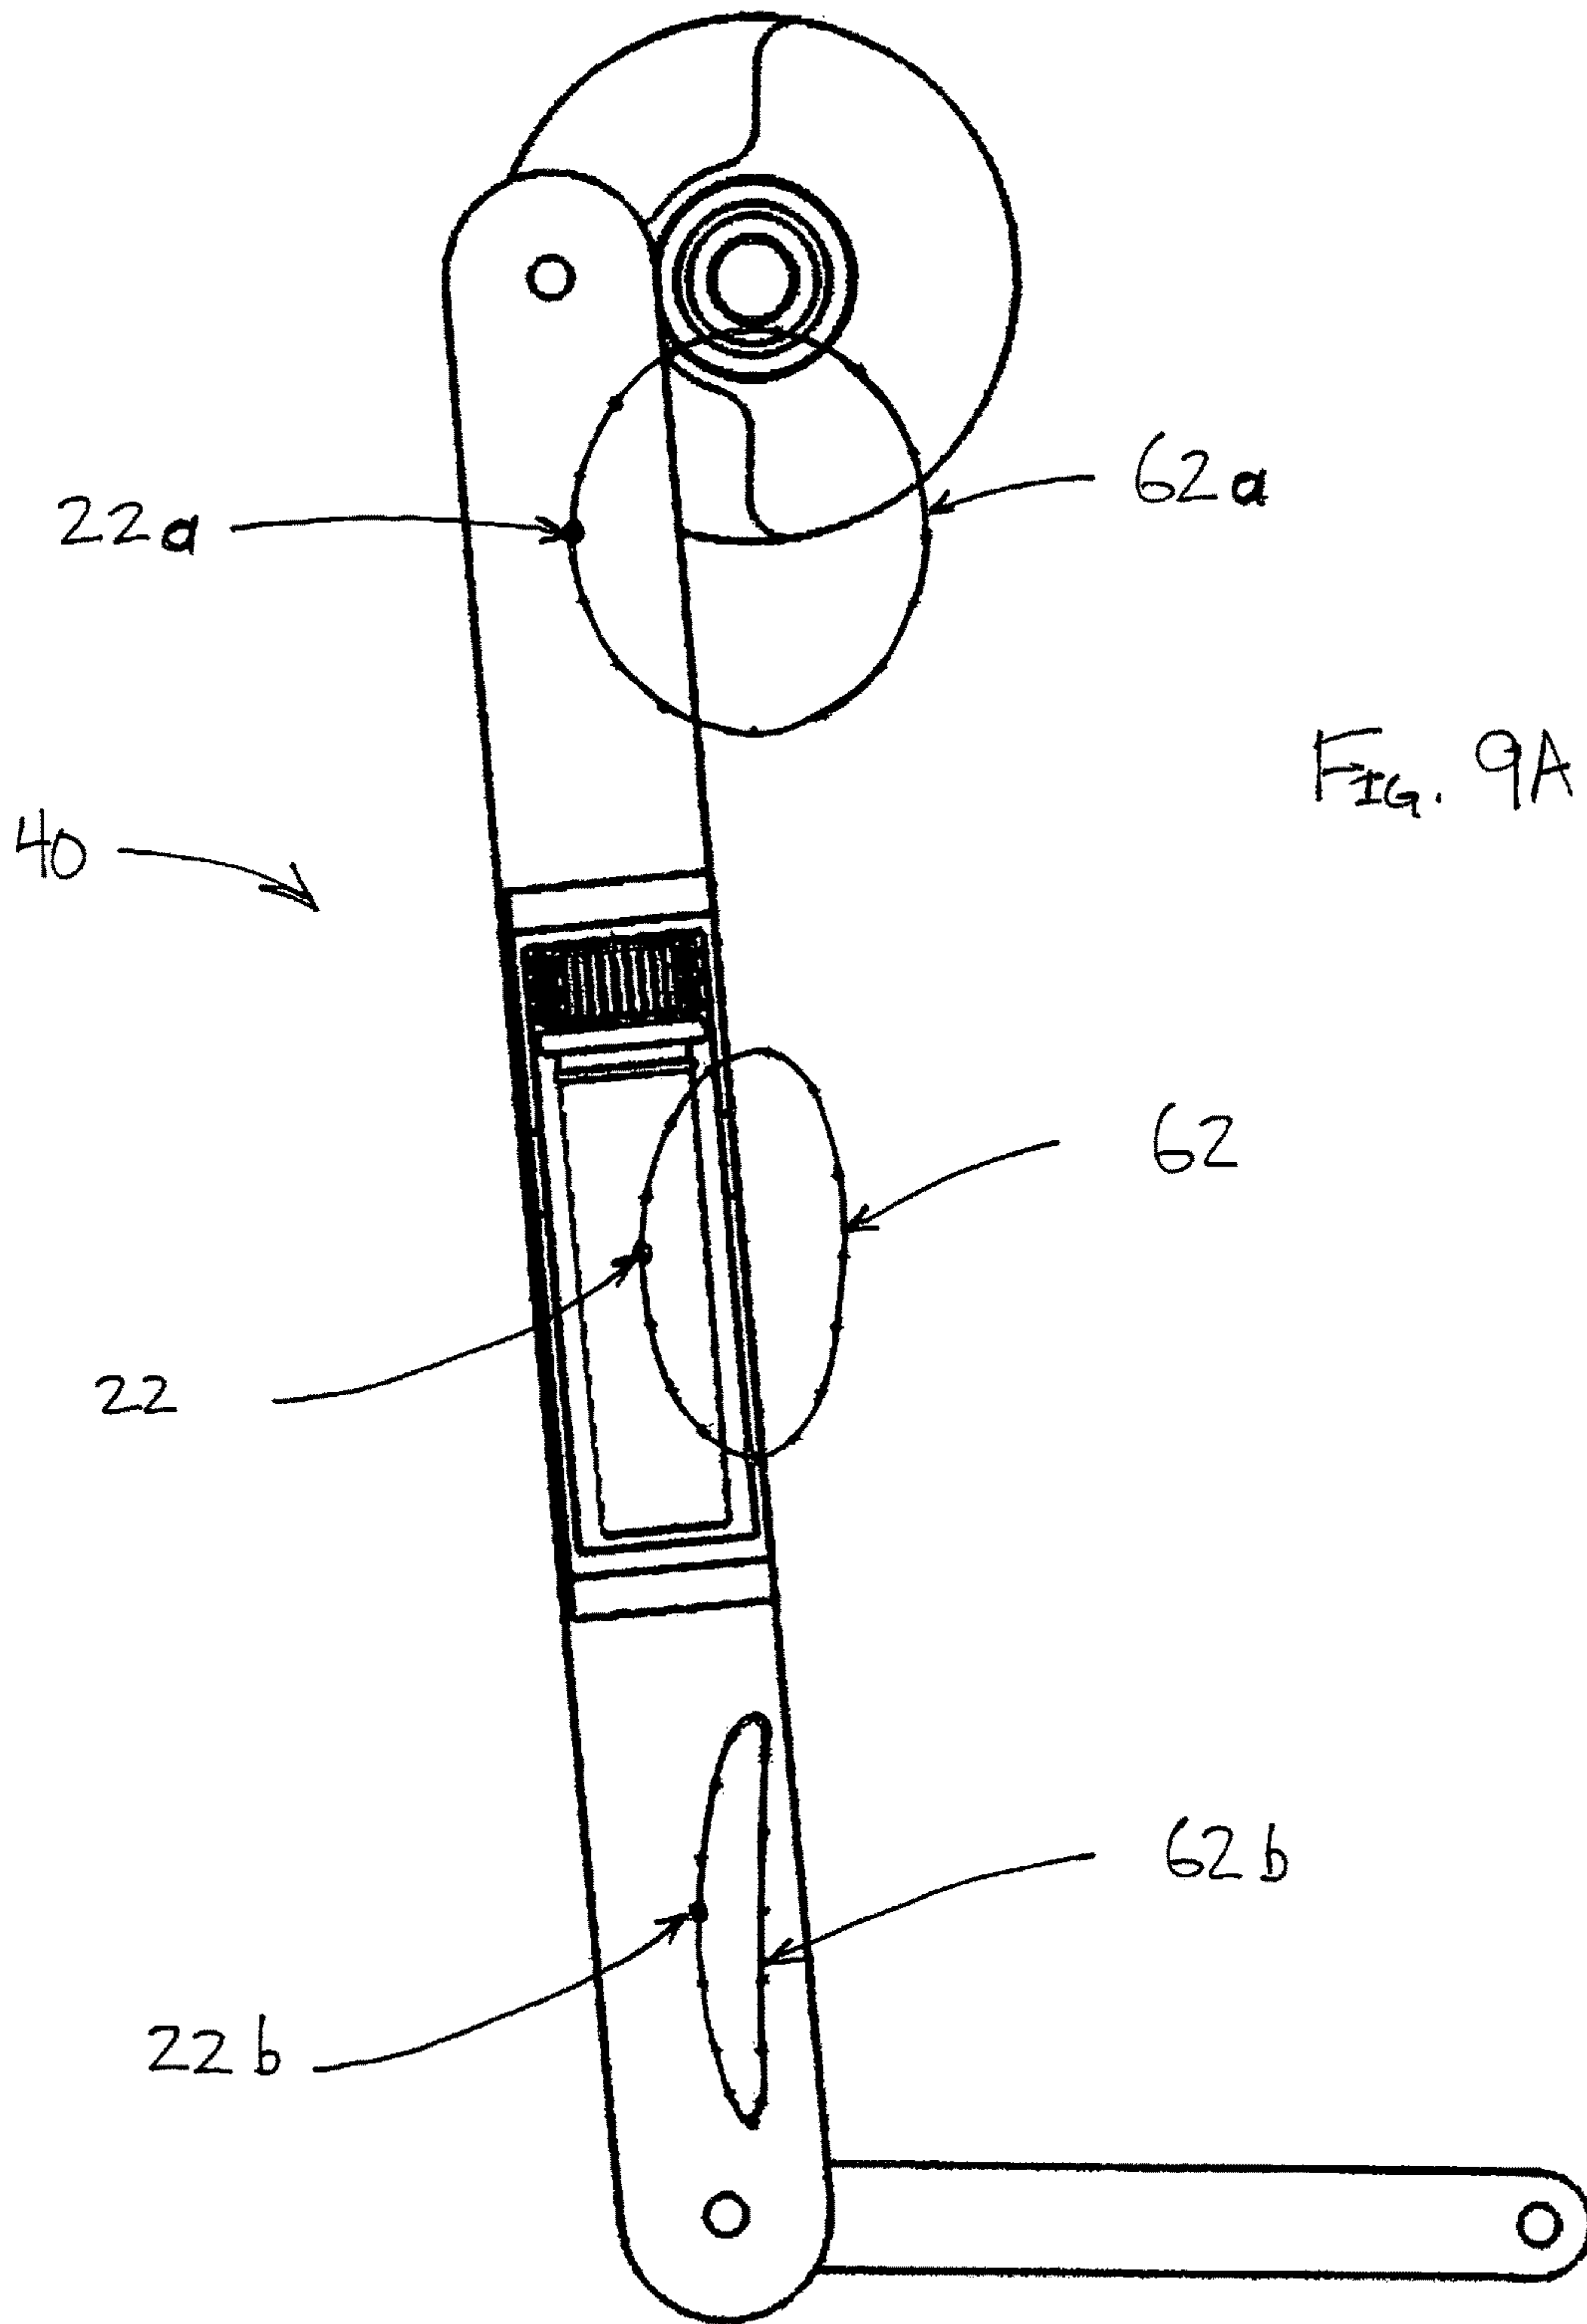



Fig. 9A

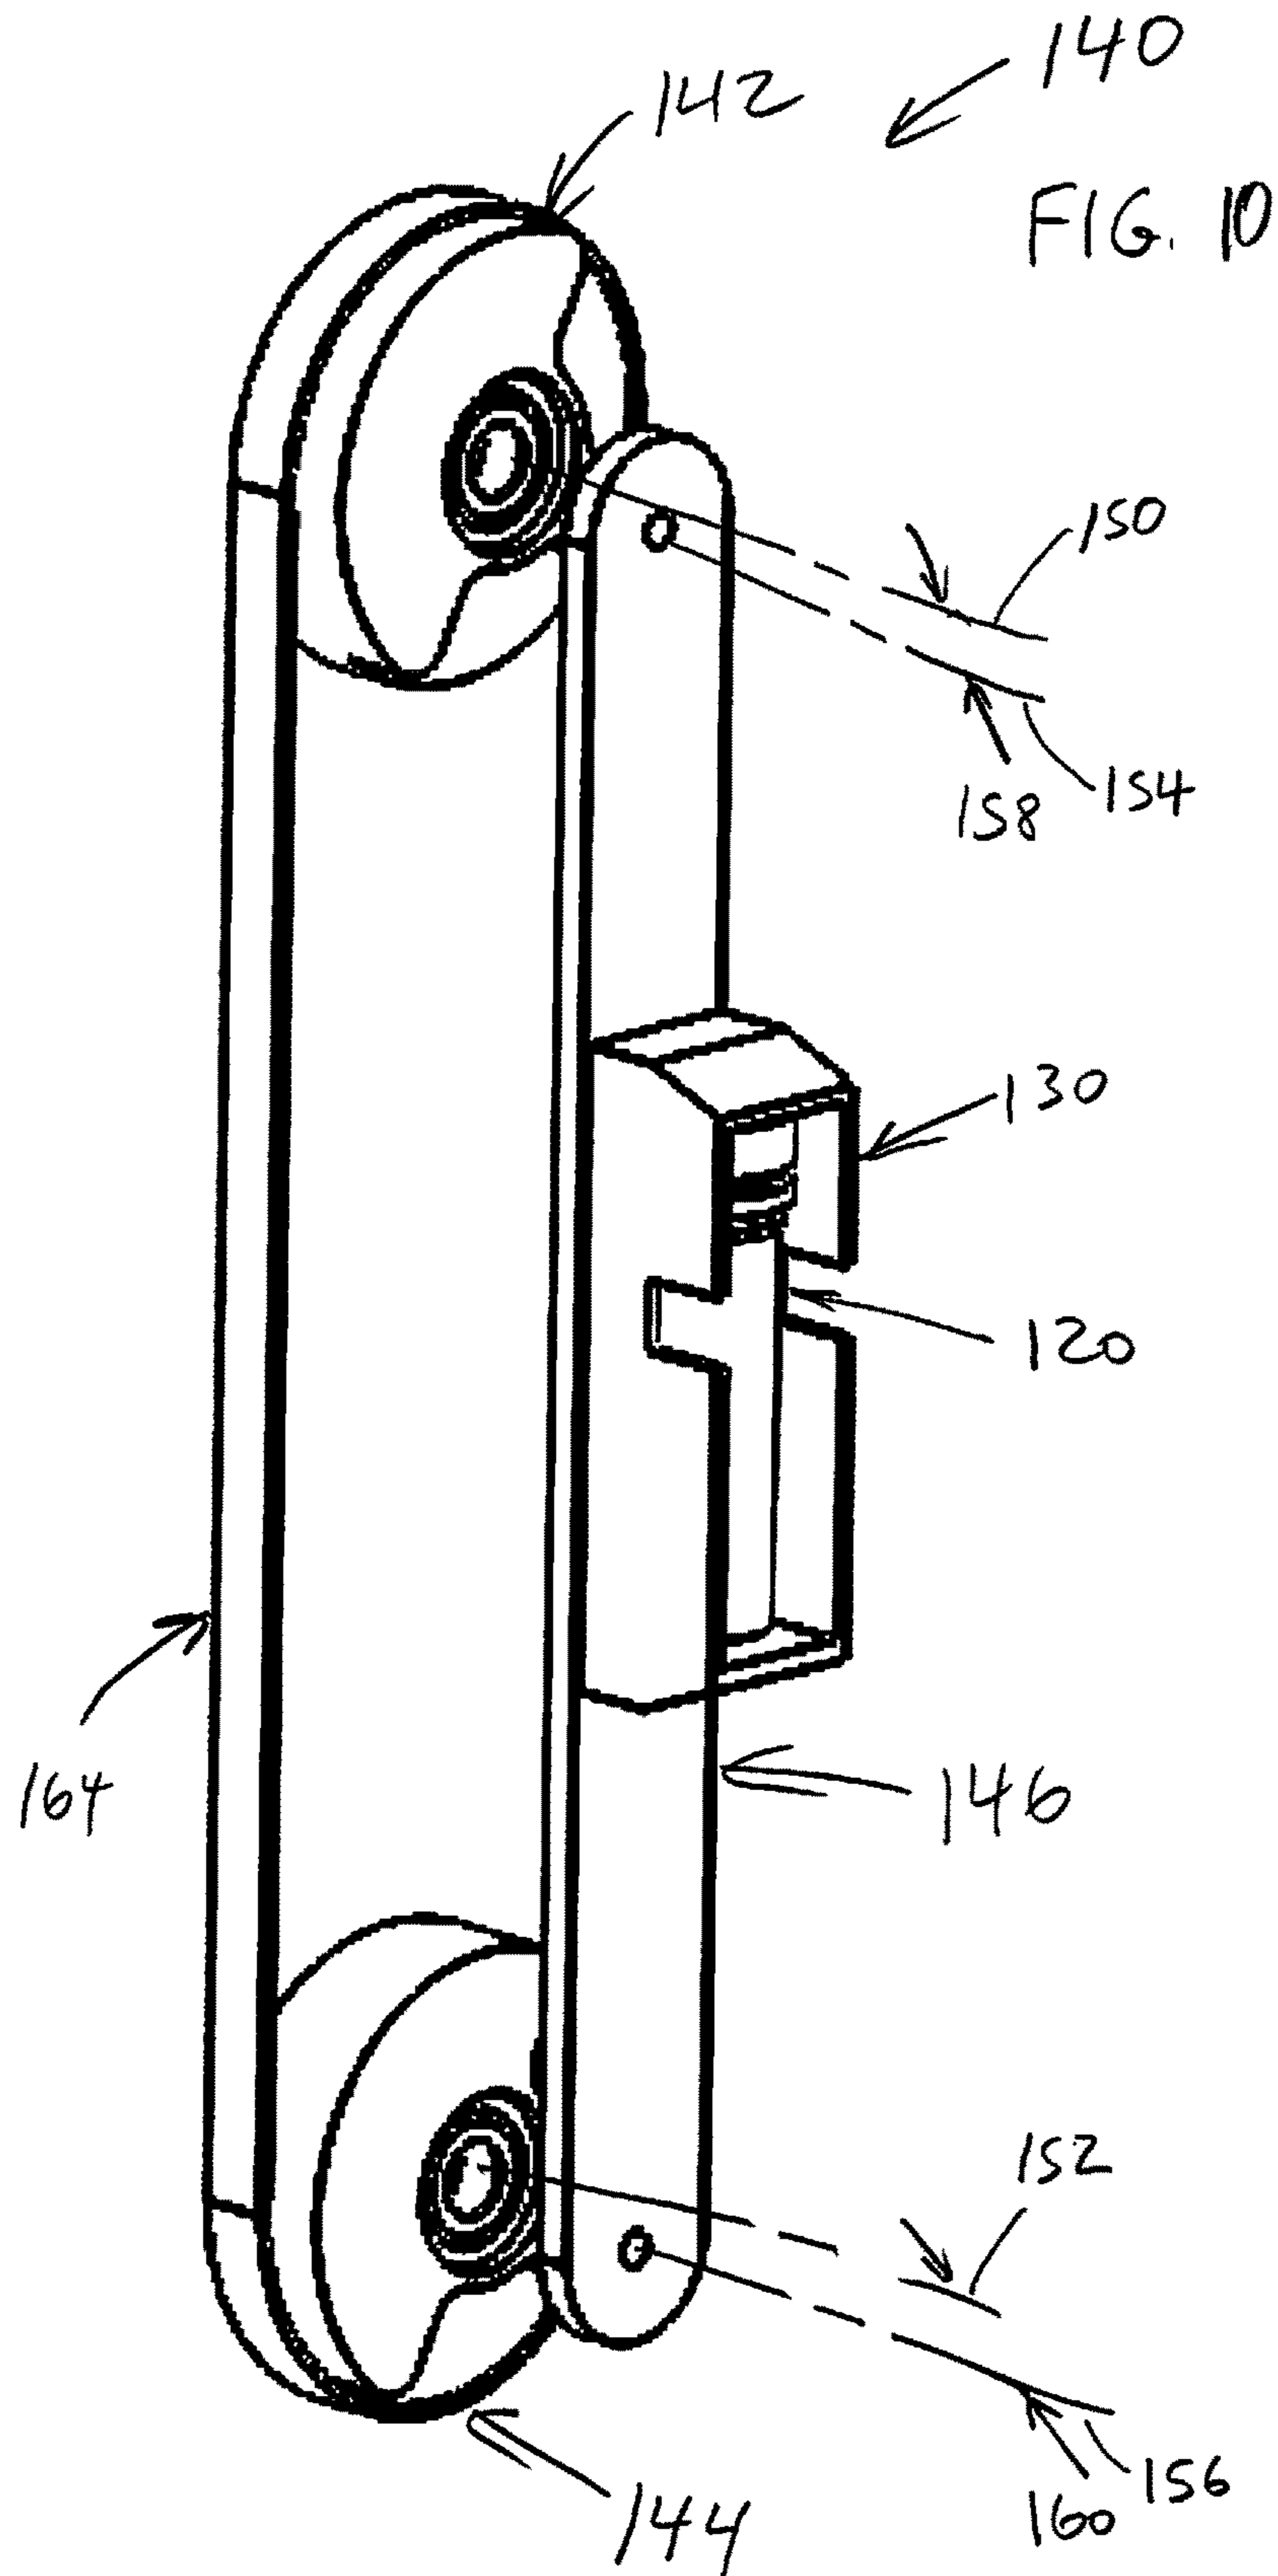

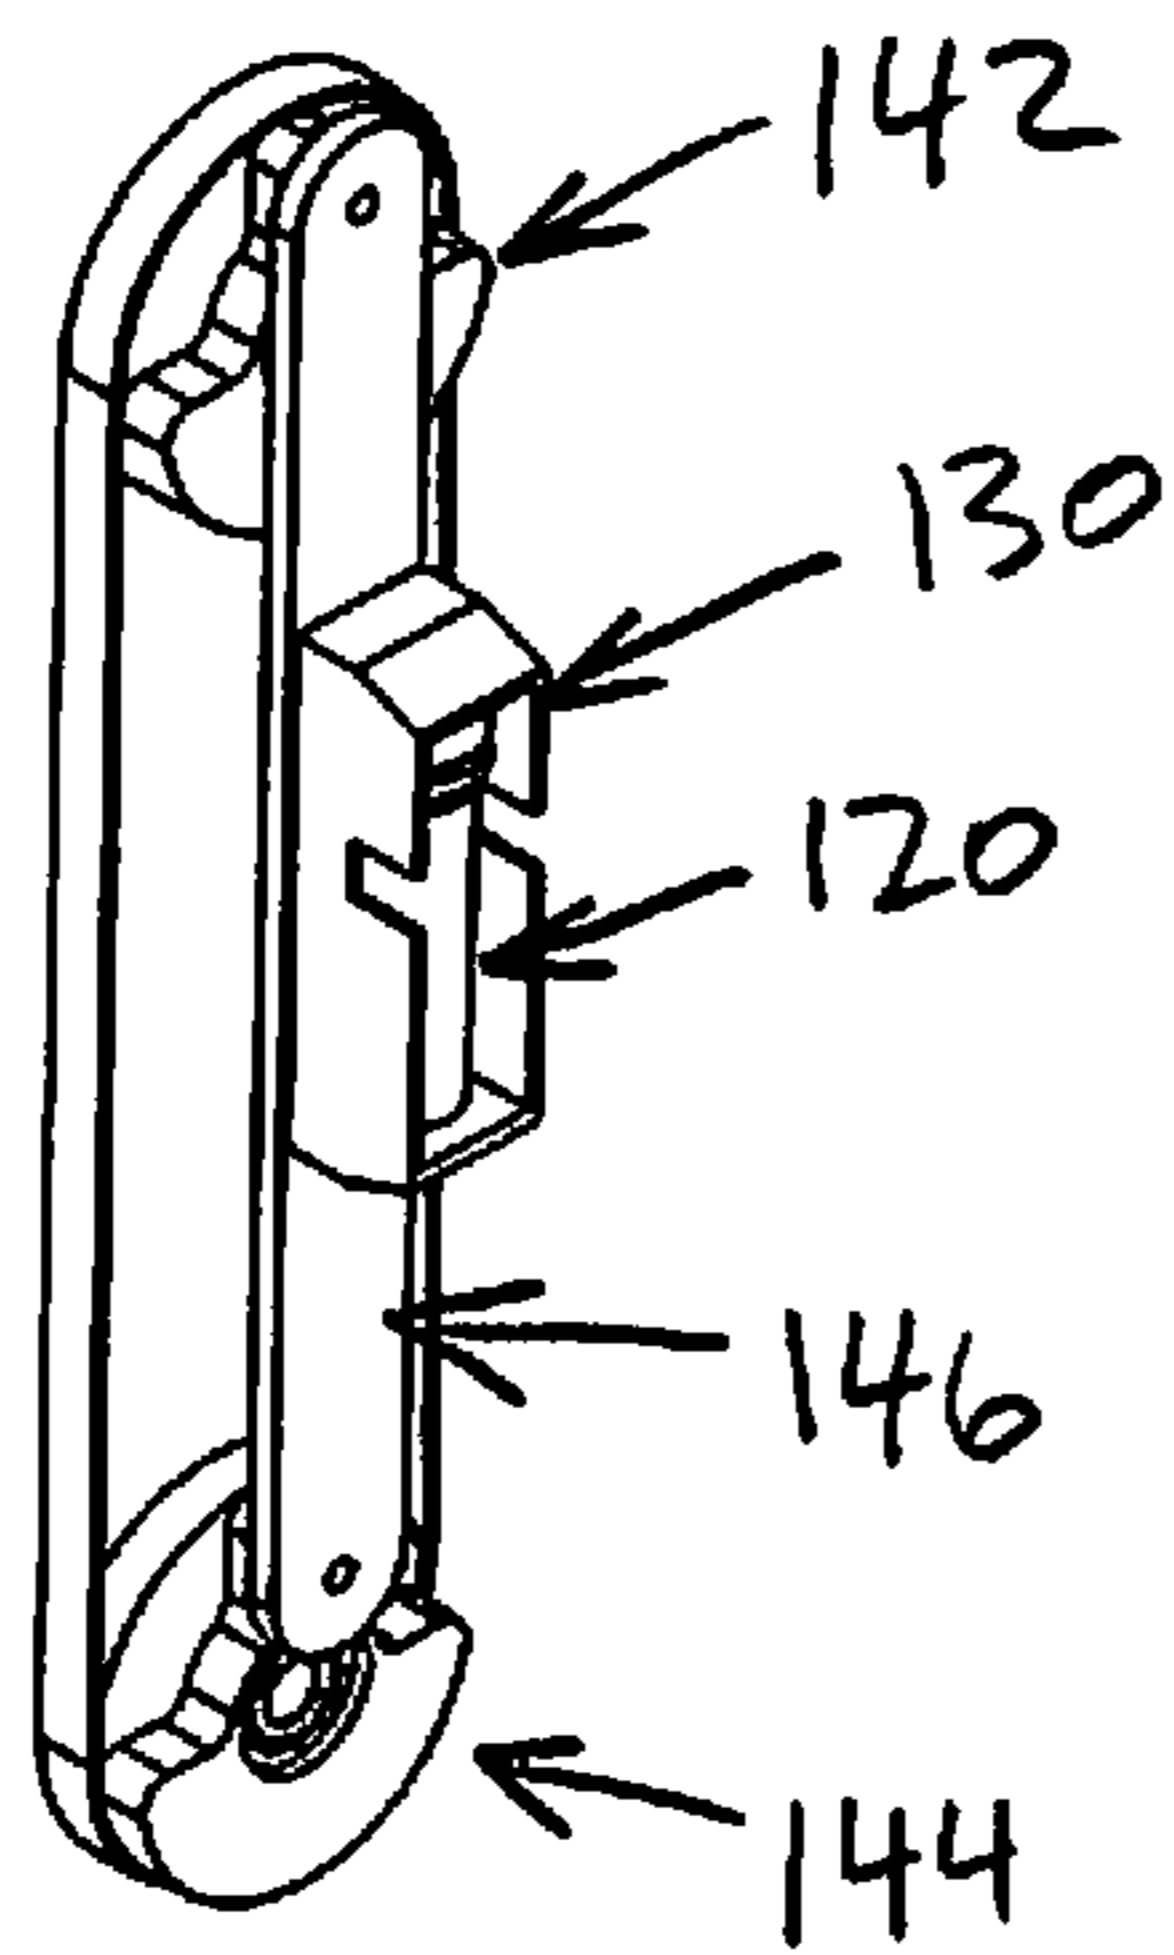


← 140

FIG. 11

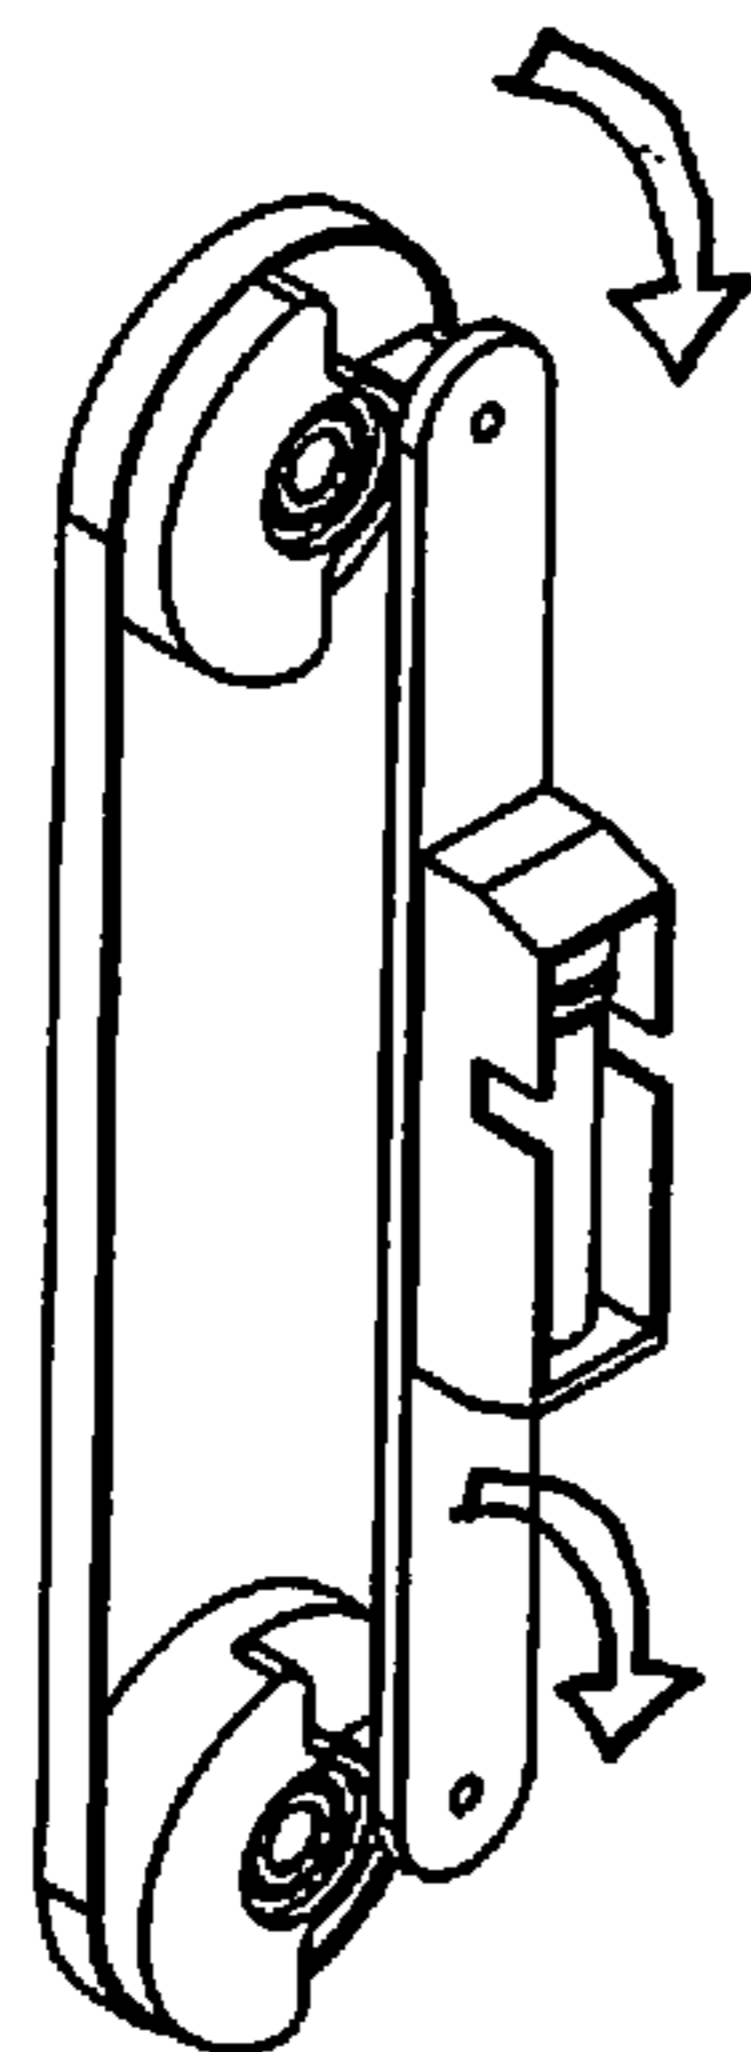


← 140

FIG. 12

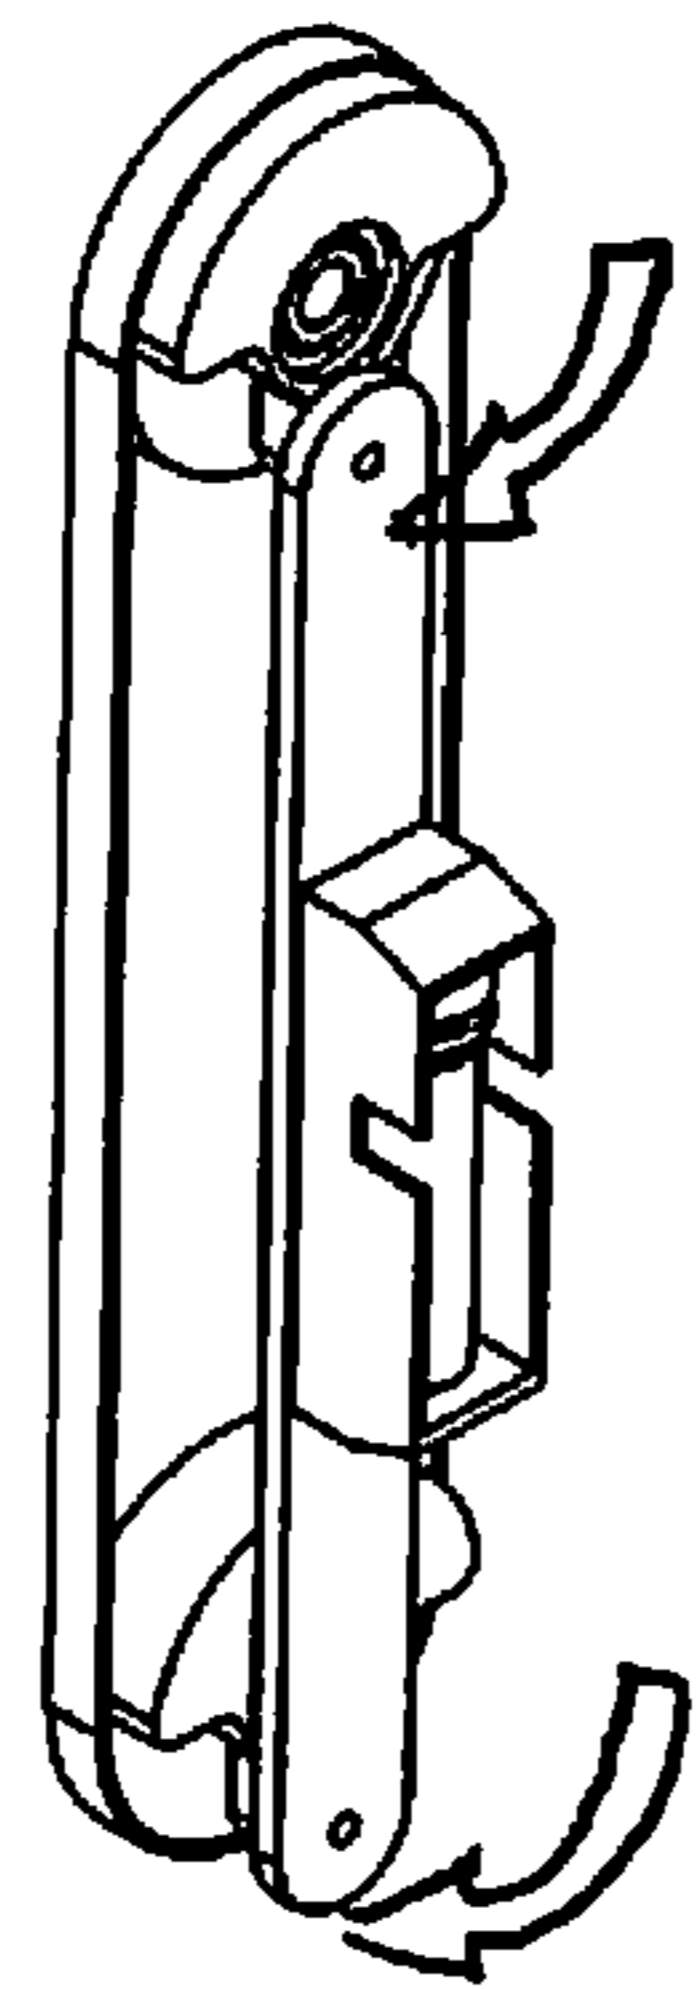


← 140

FIG. 13

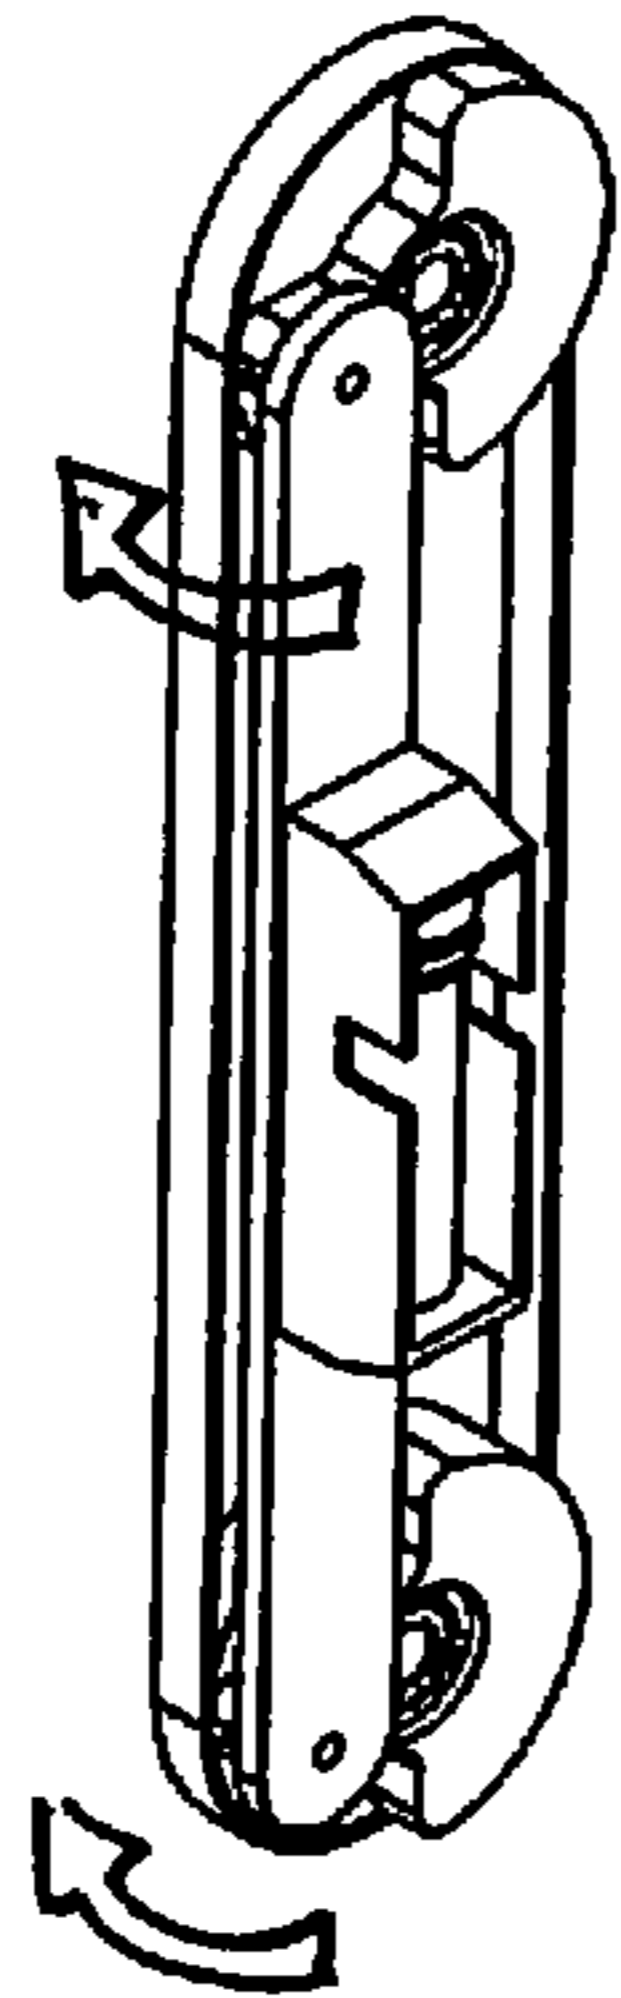


← 140

FIG. 14

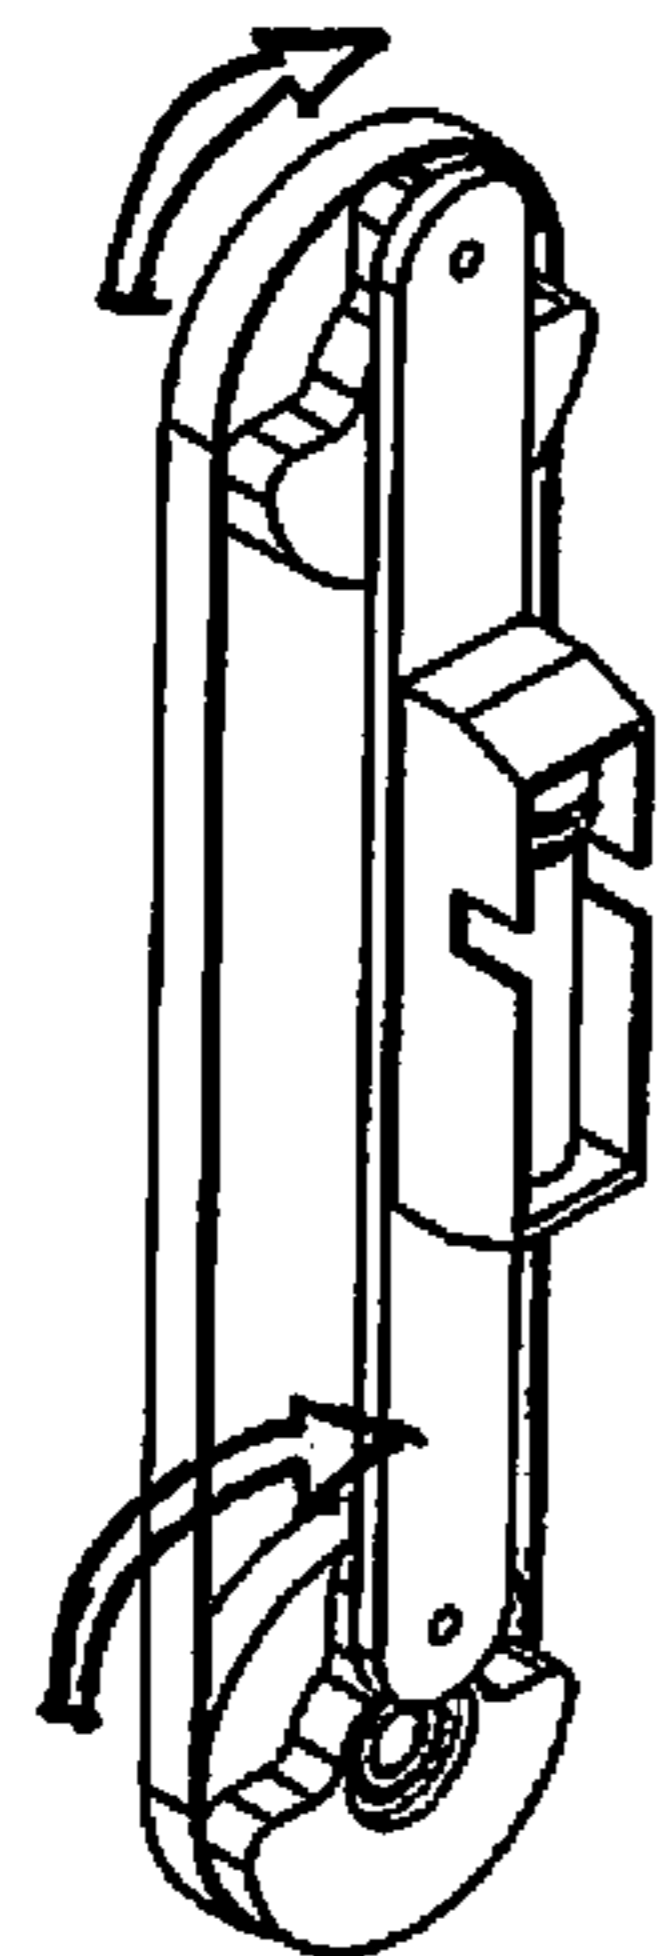


← 140

FIG. 15

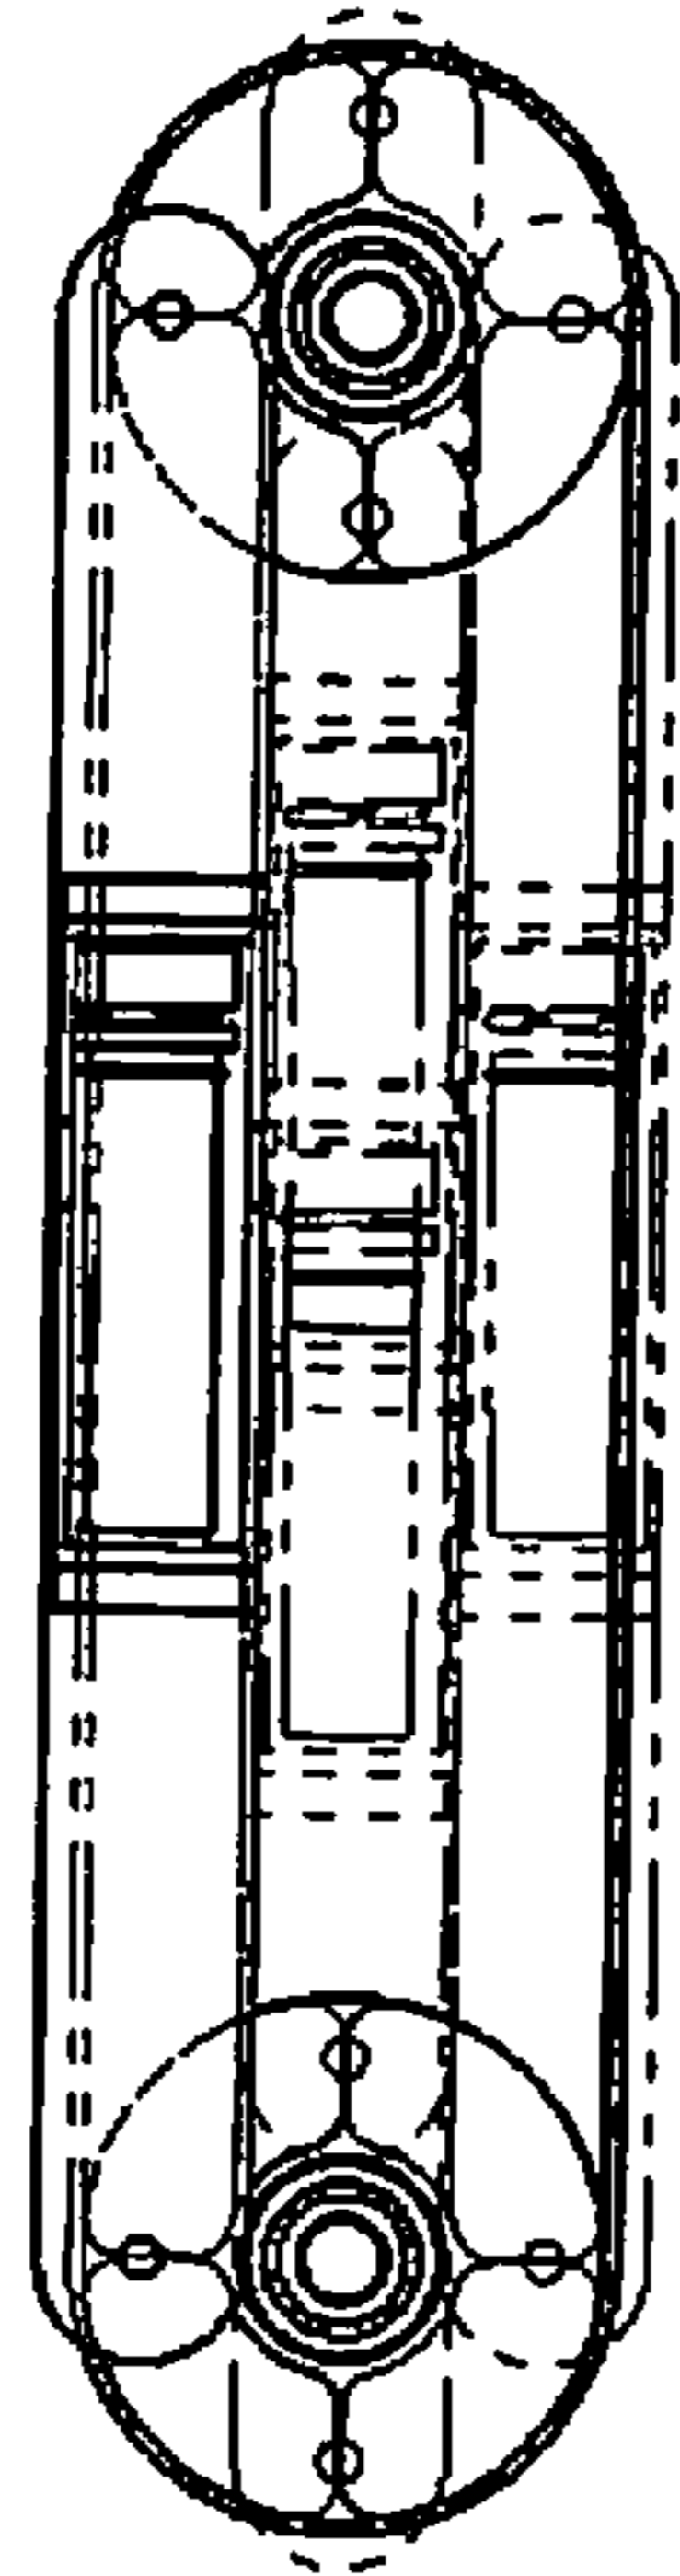


← 140


FIG. 16


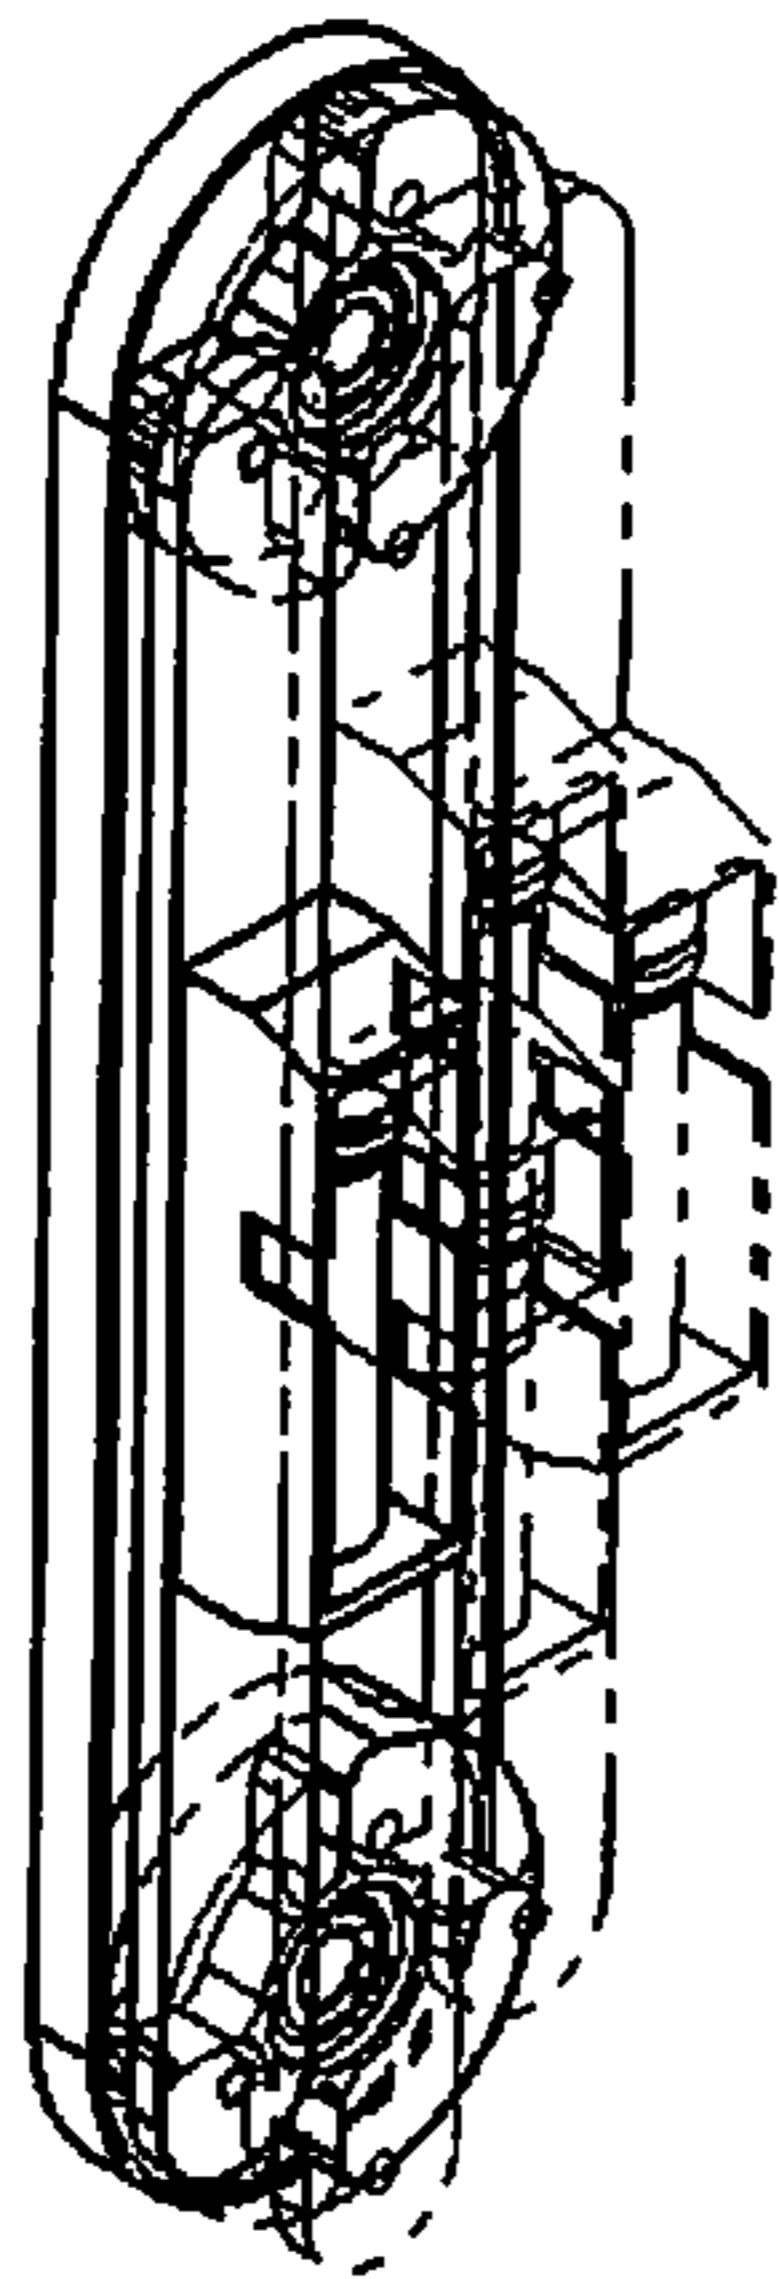



← 140

FIG. 17

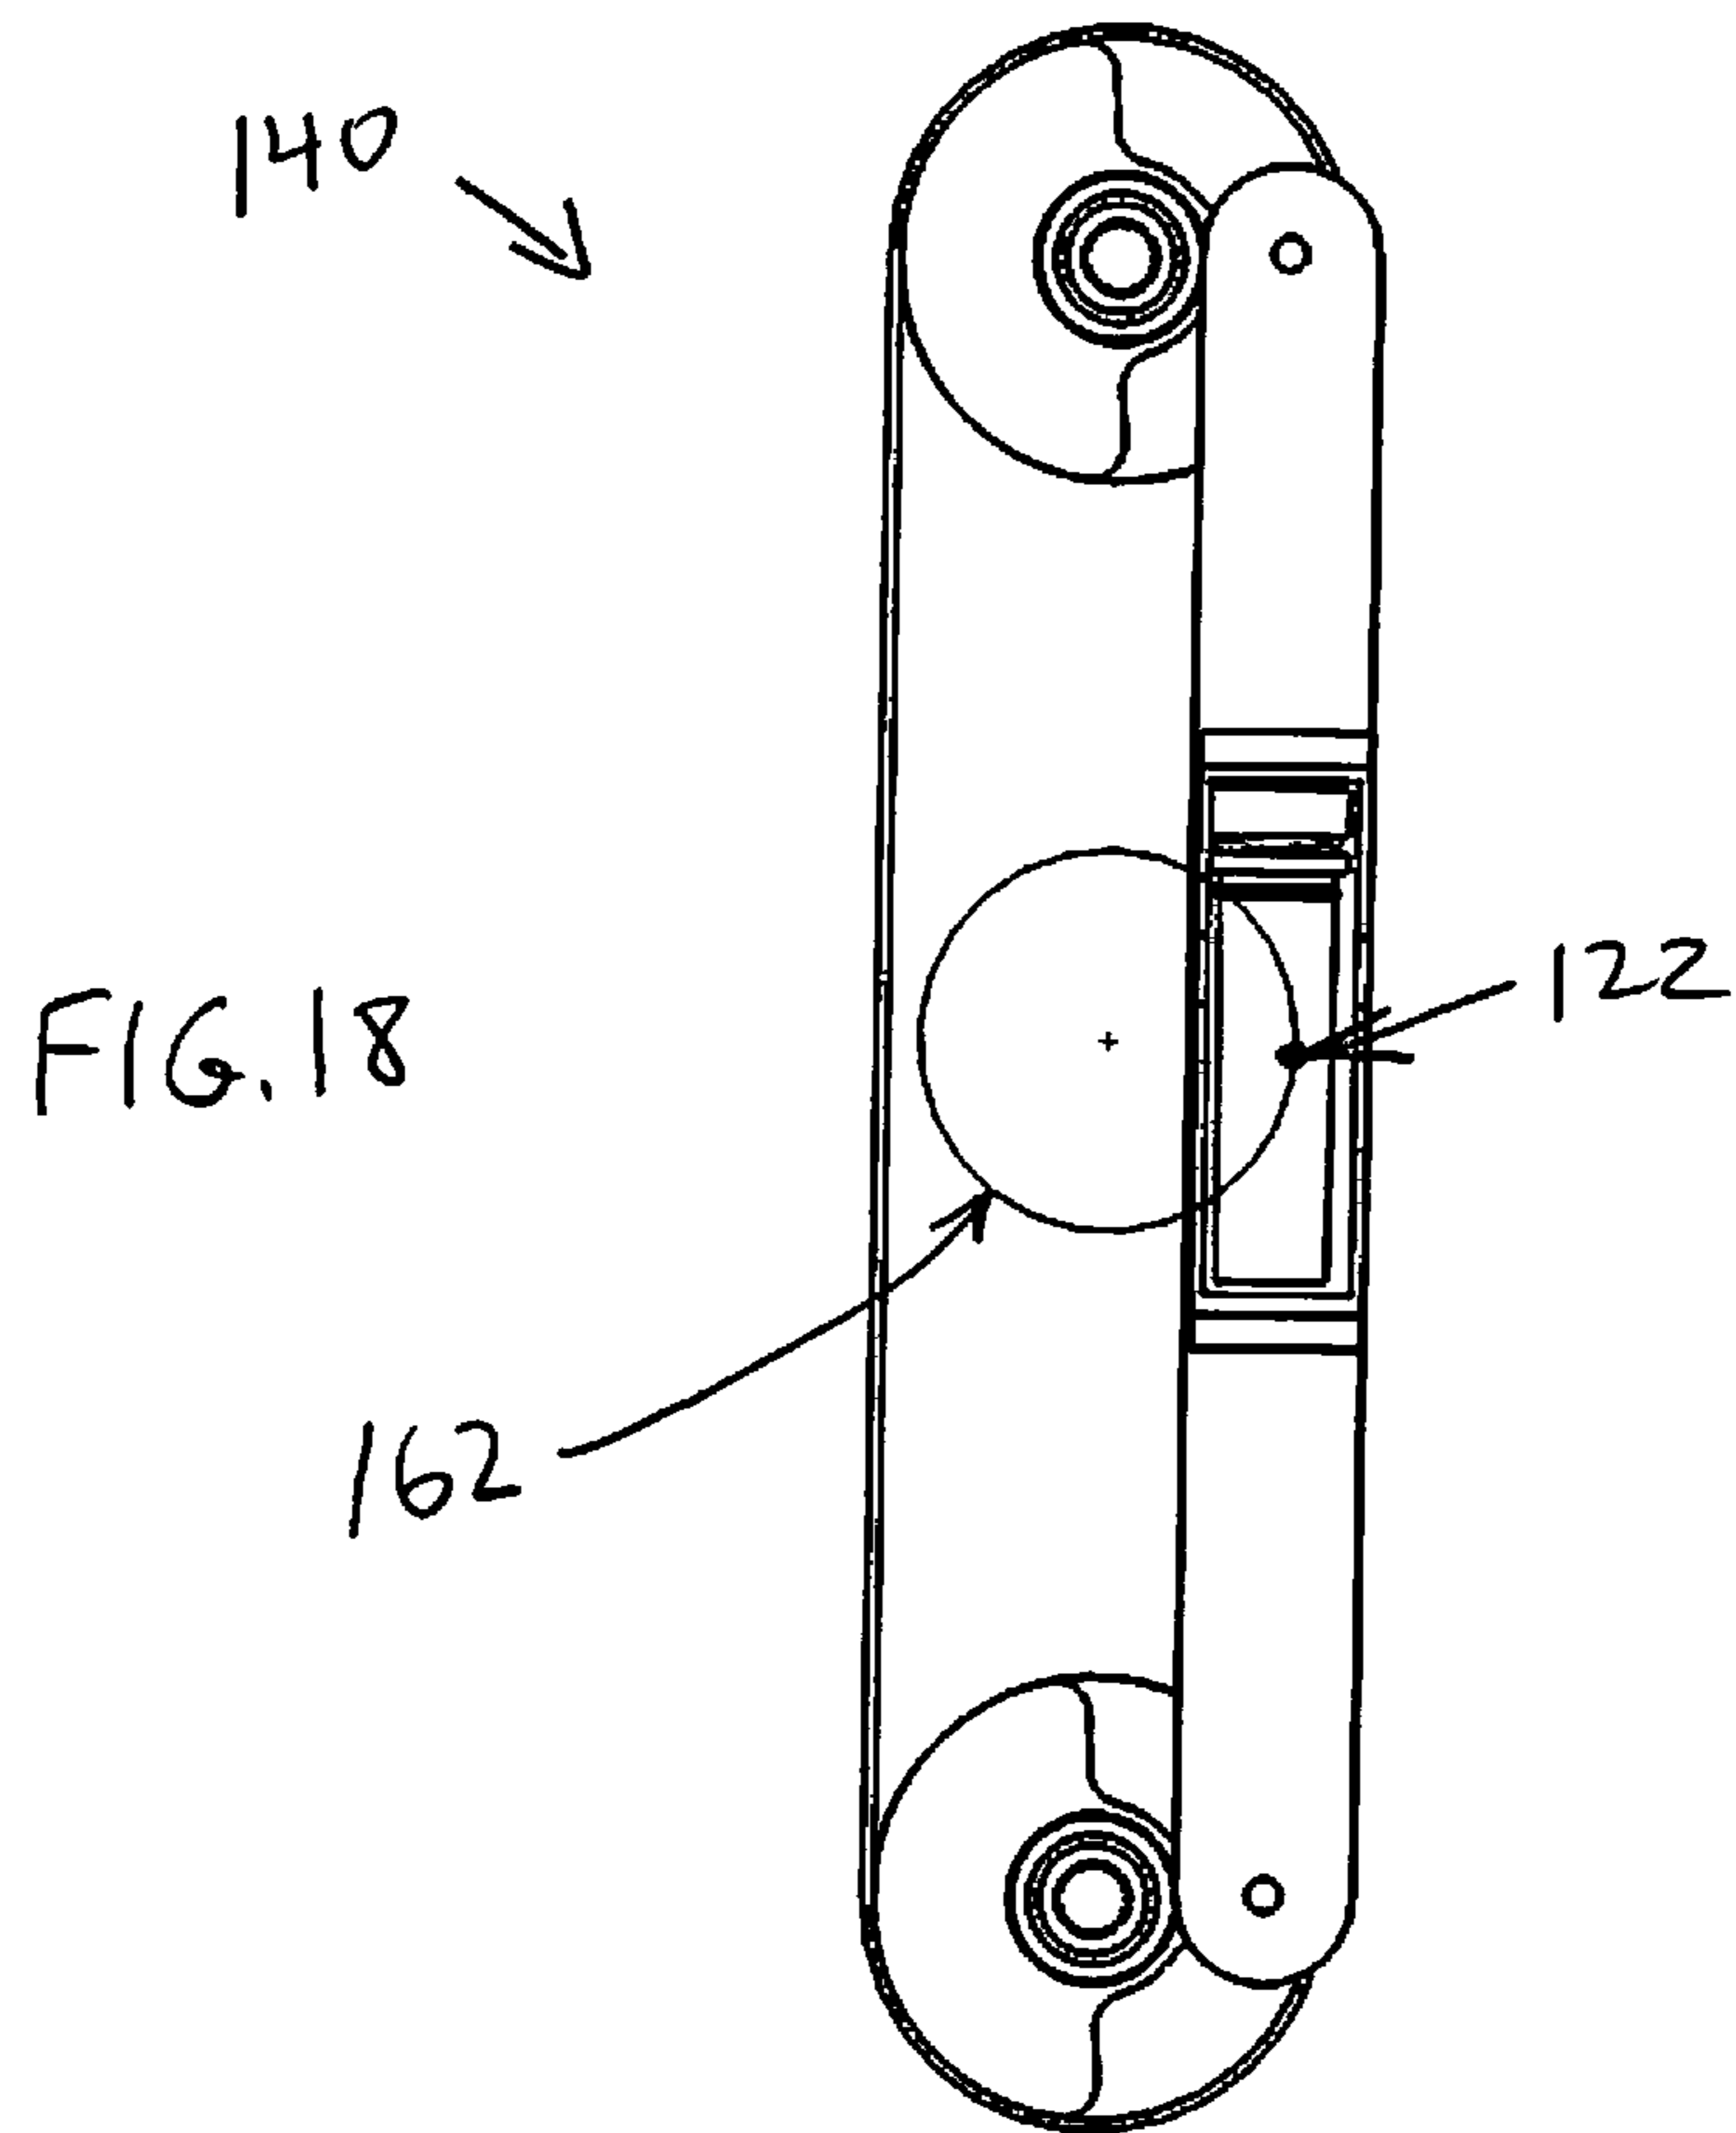

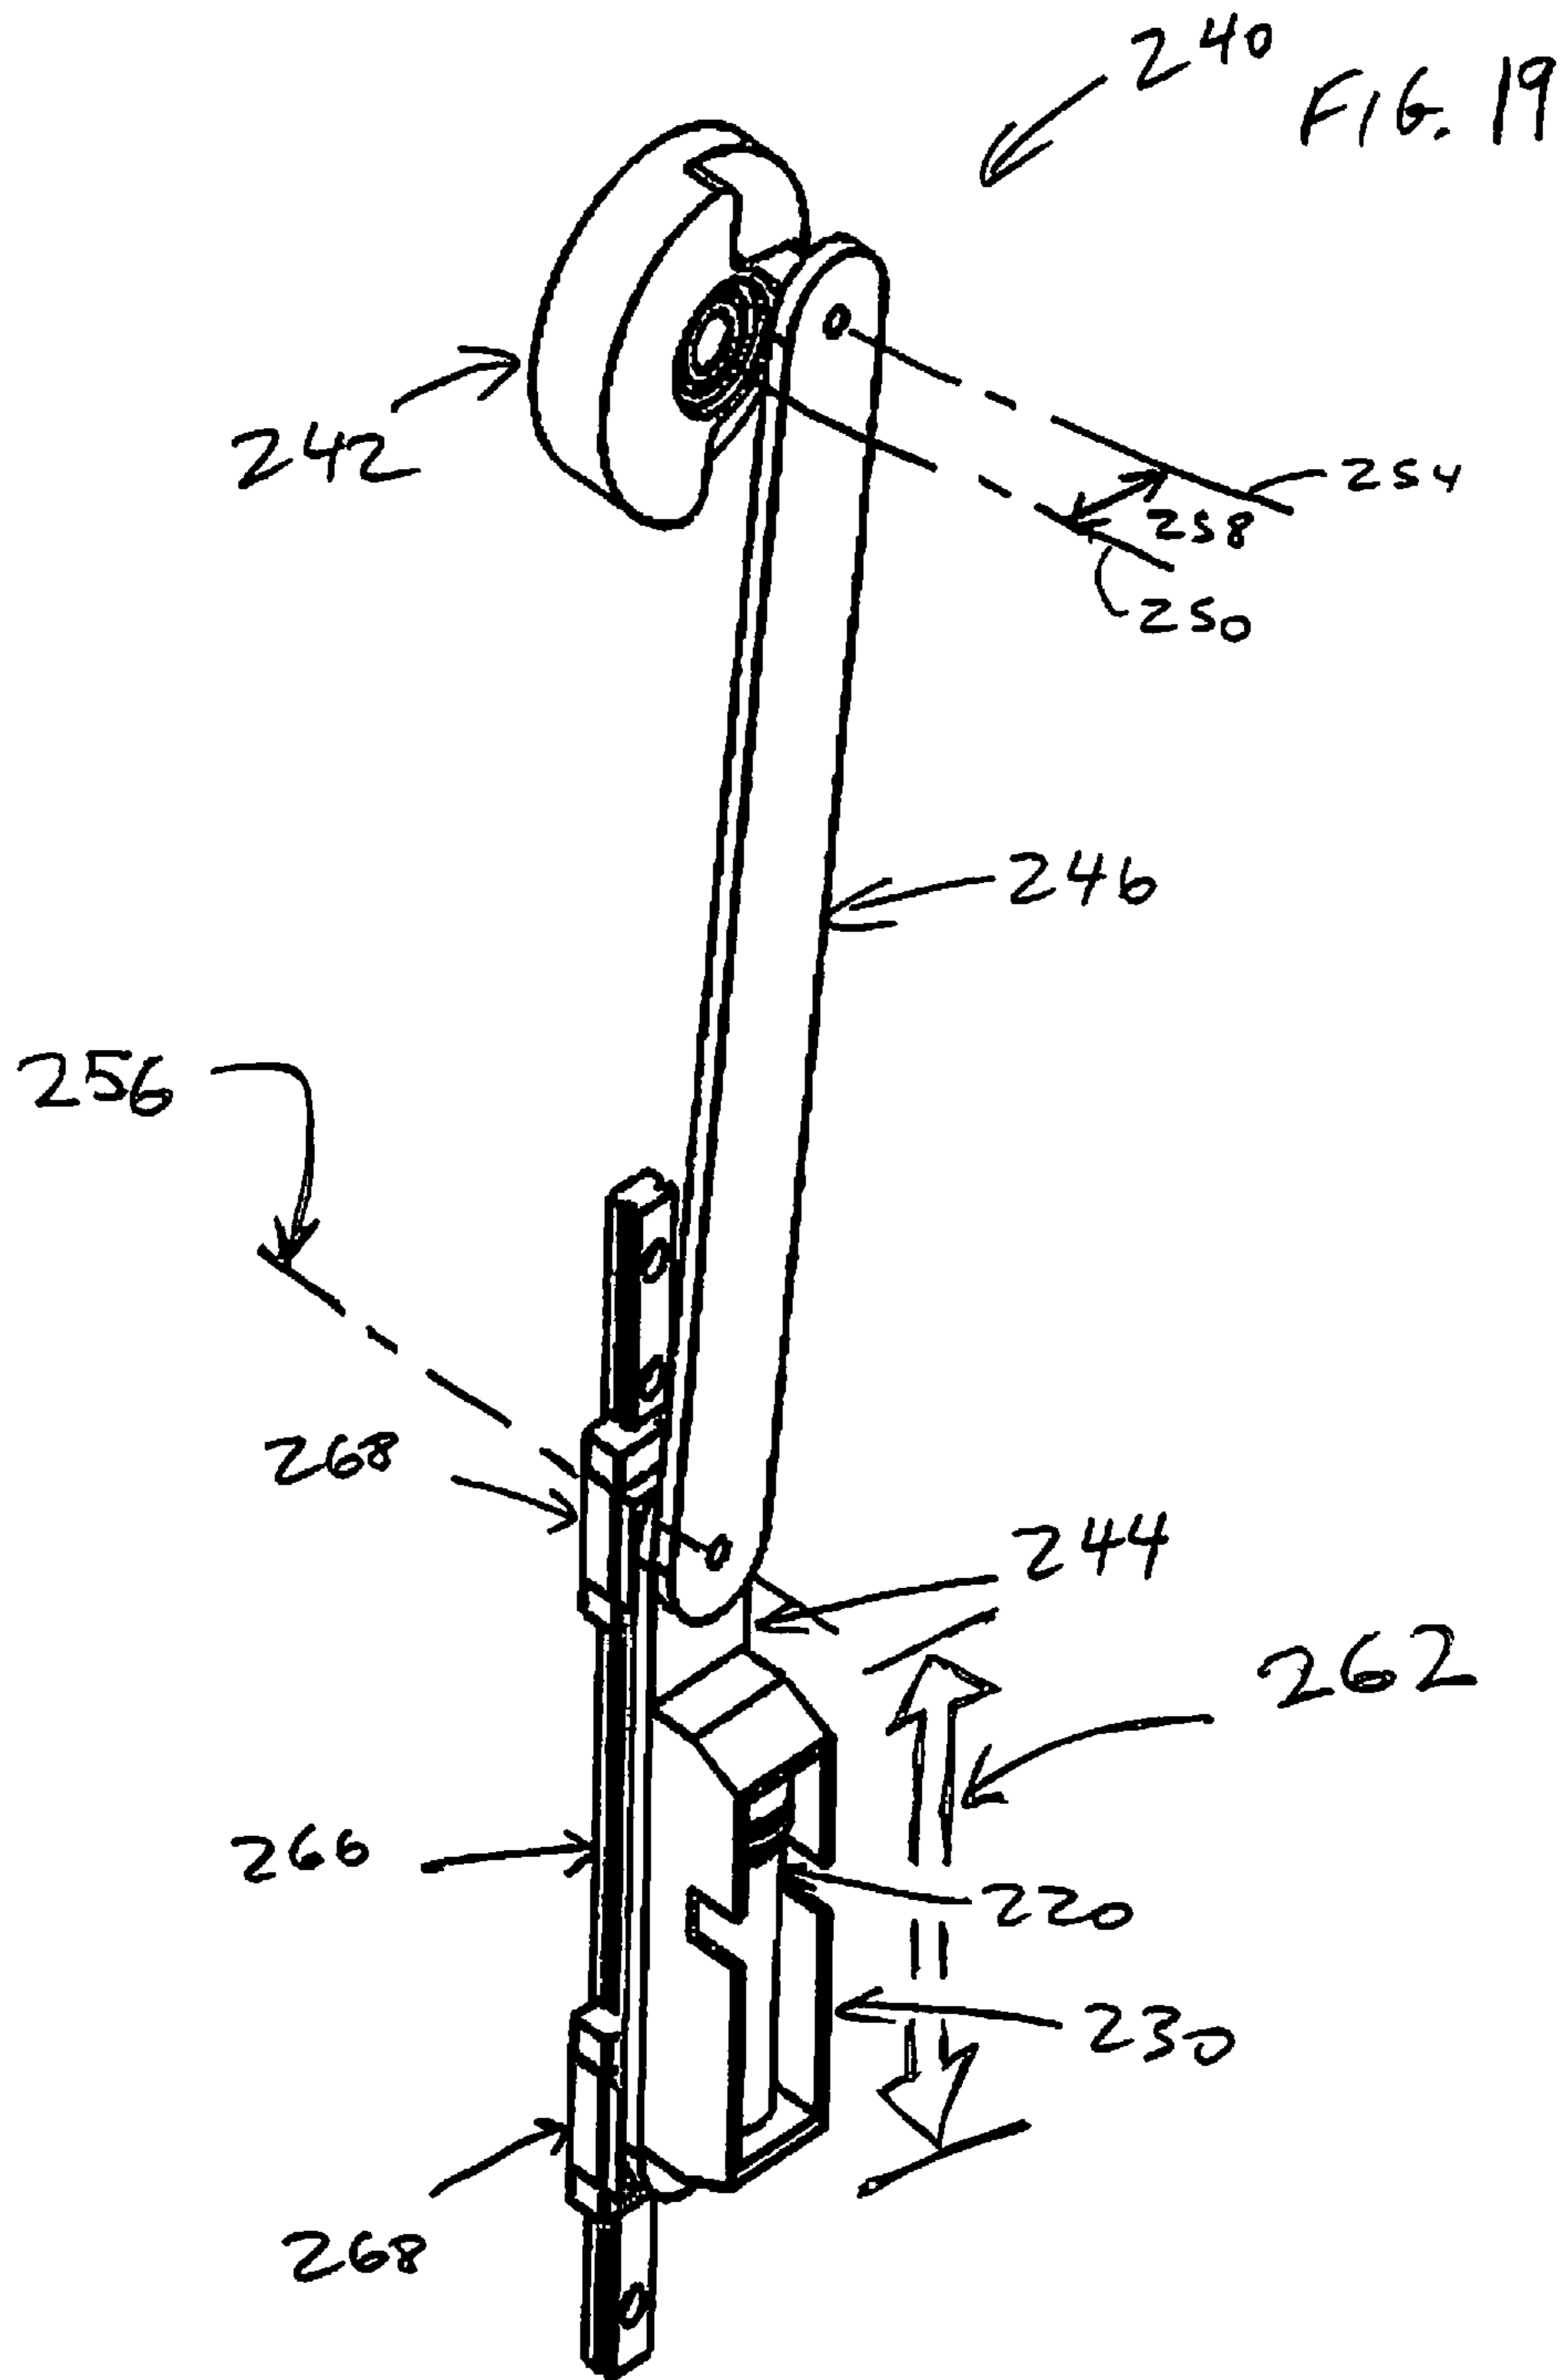


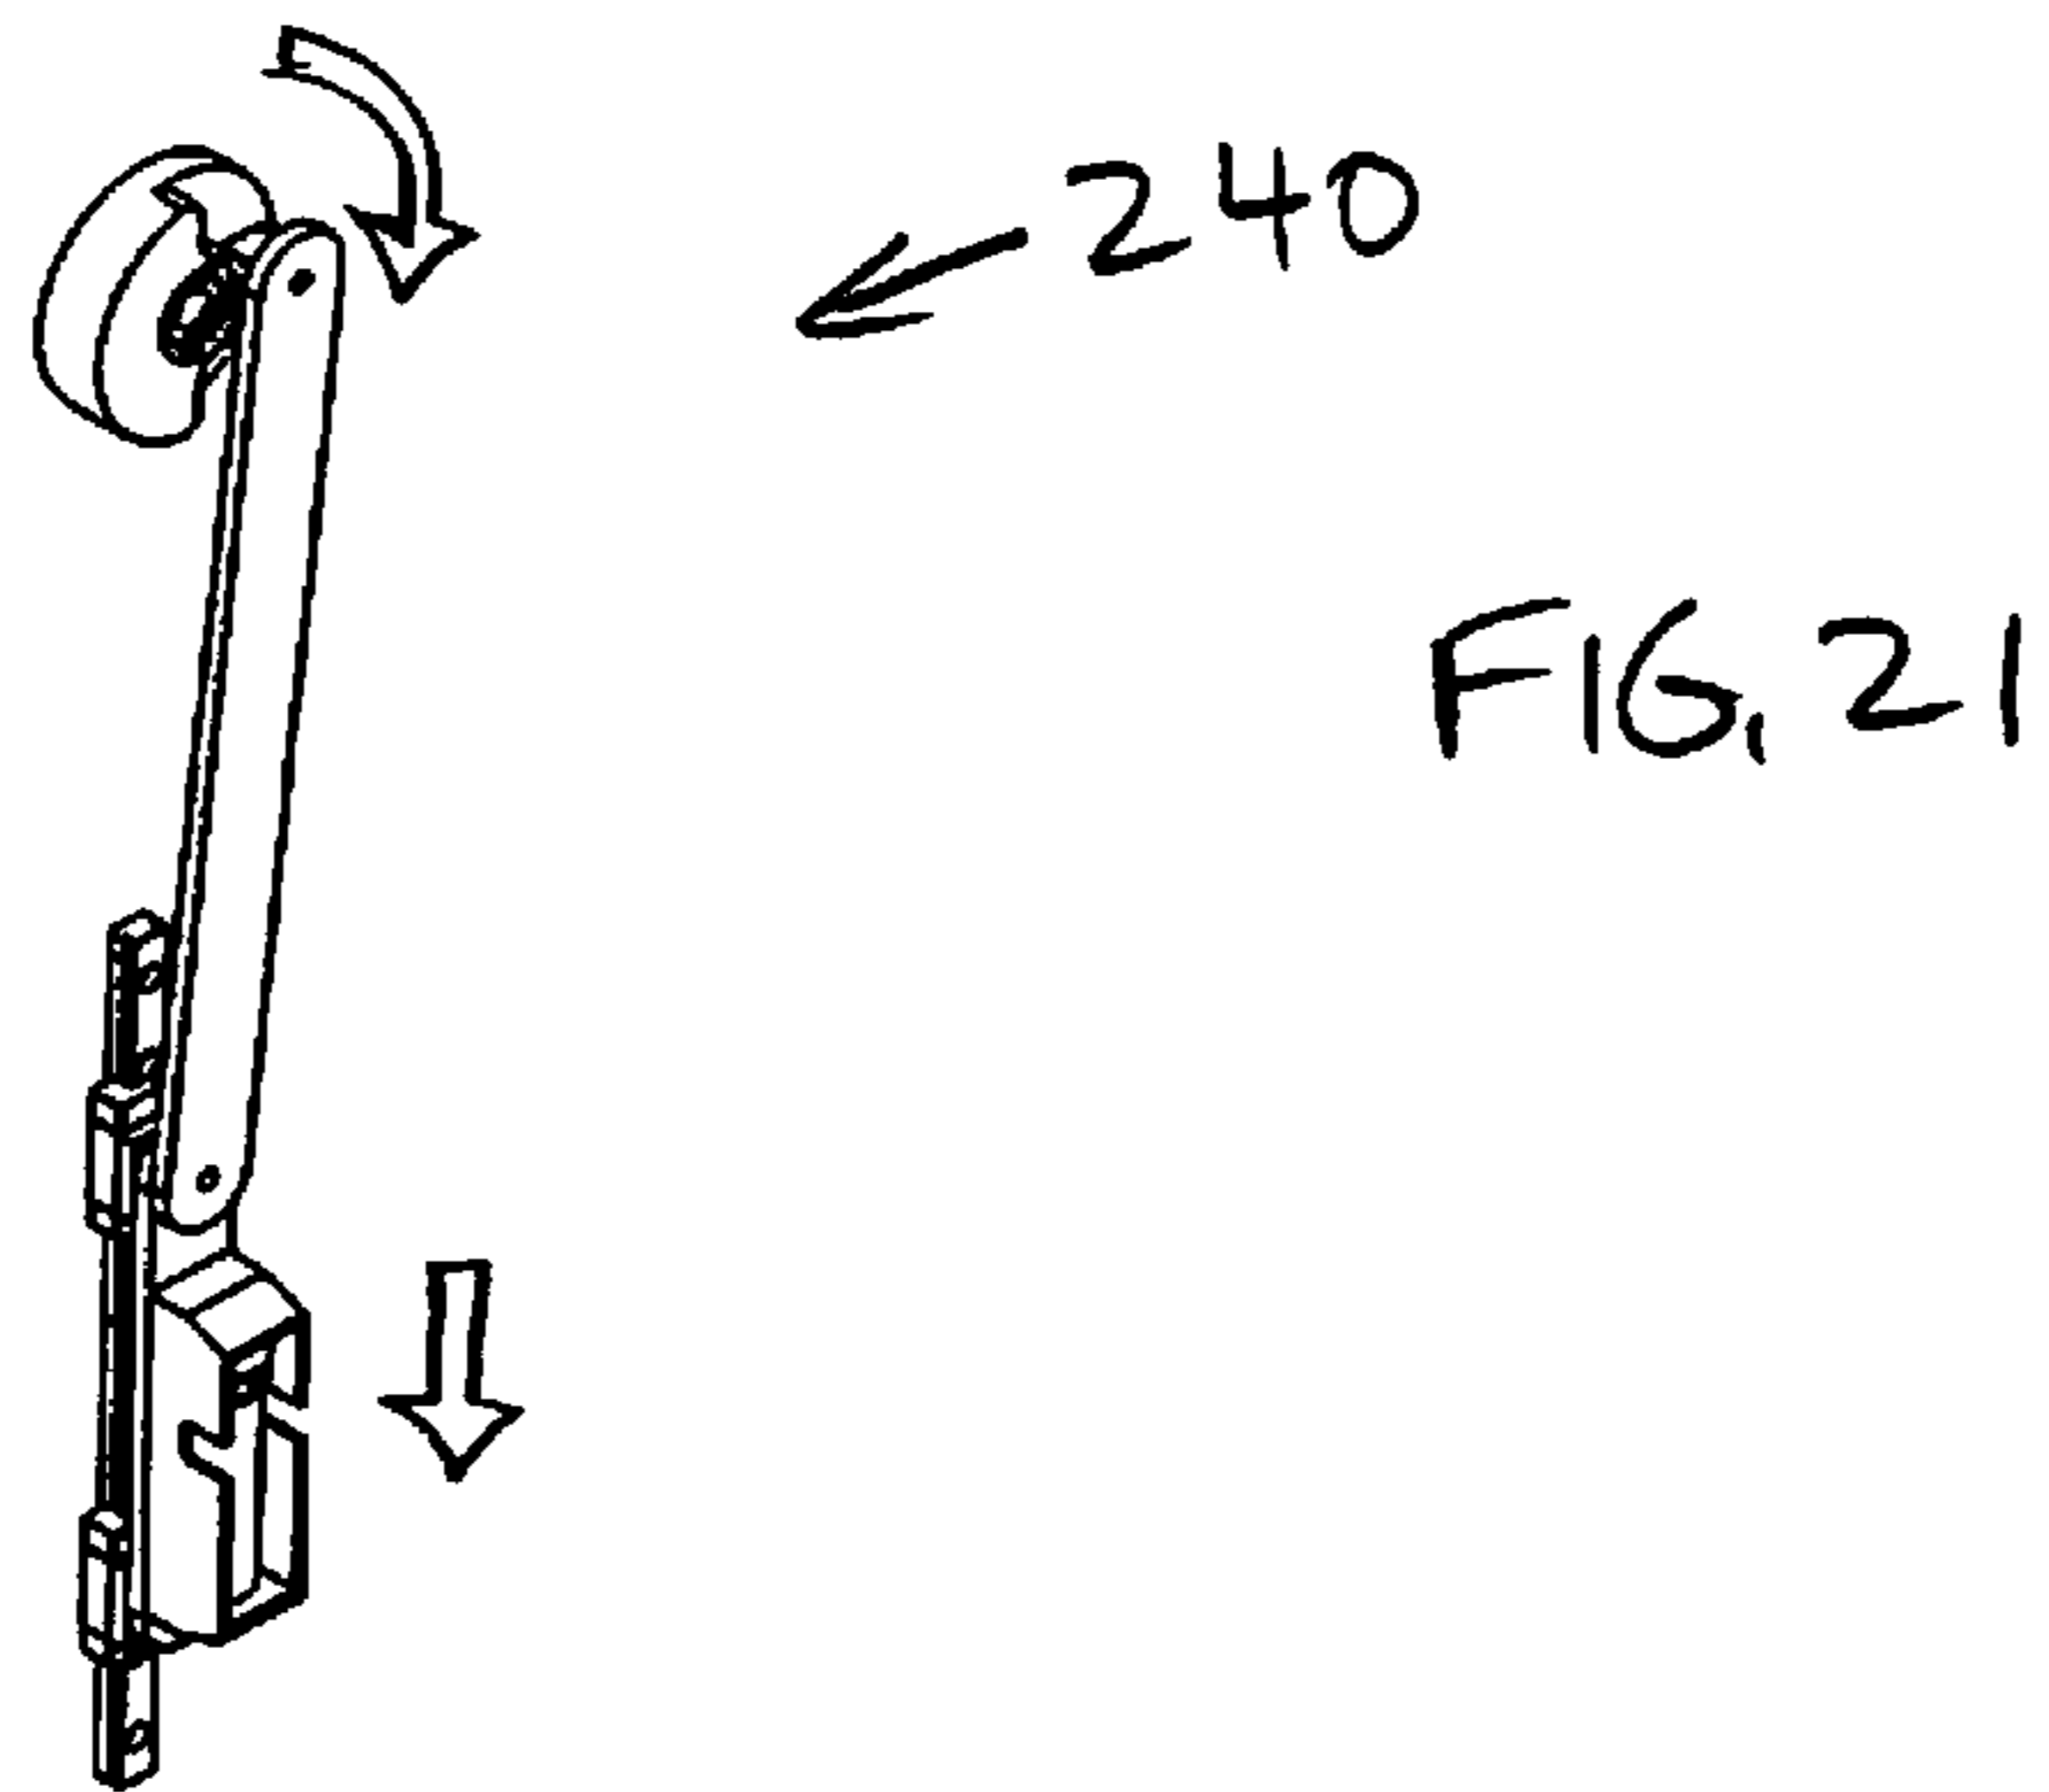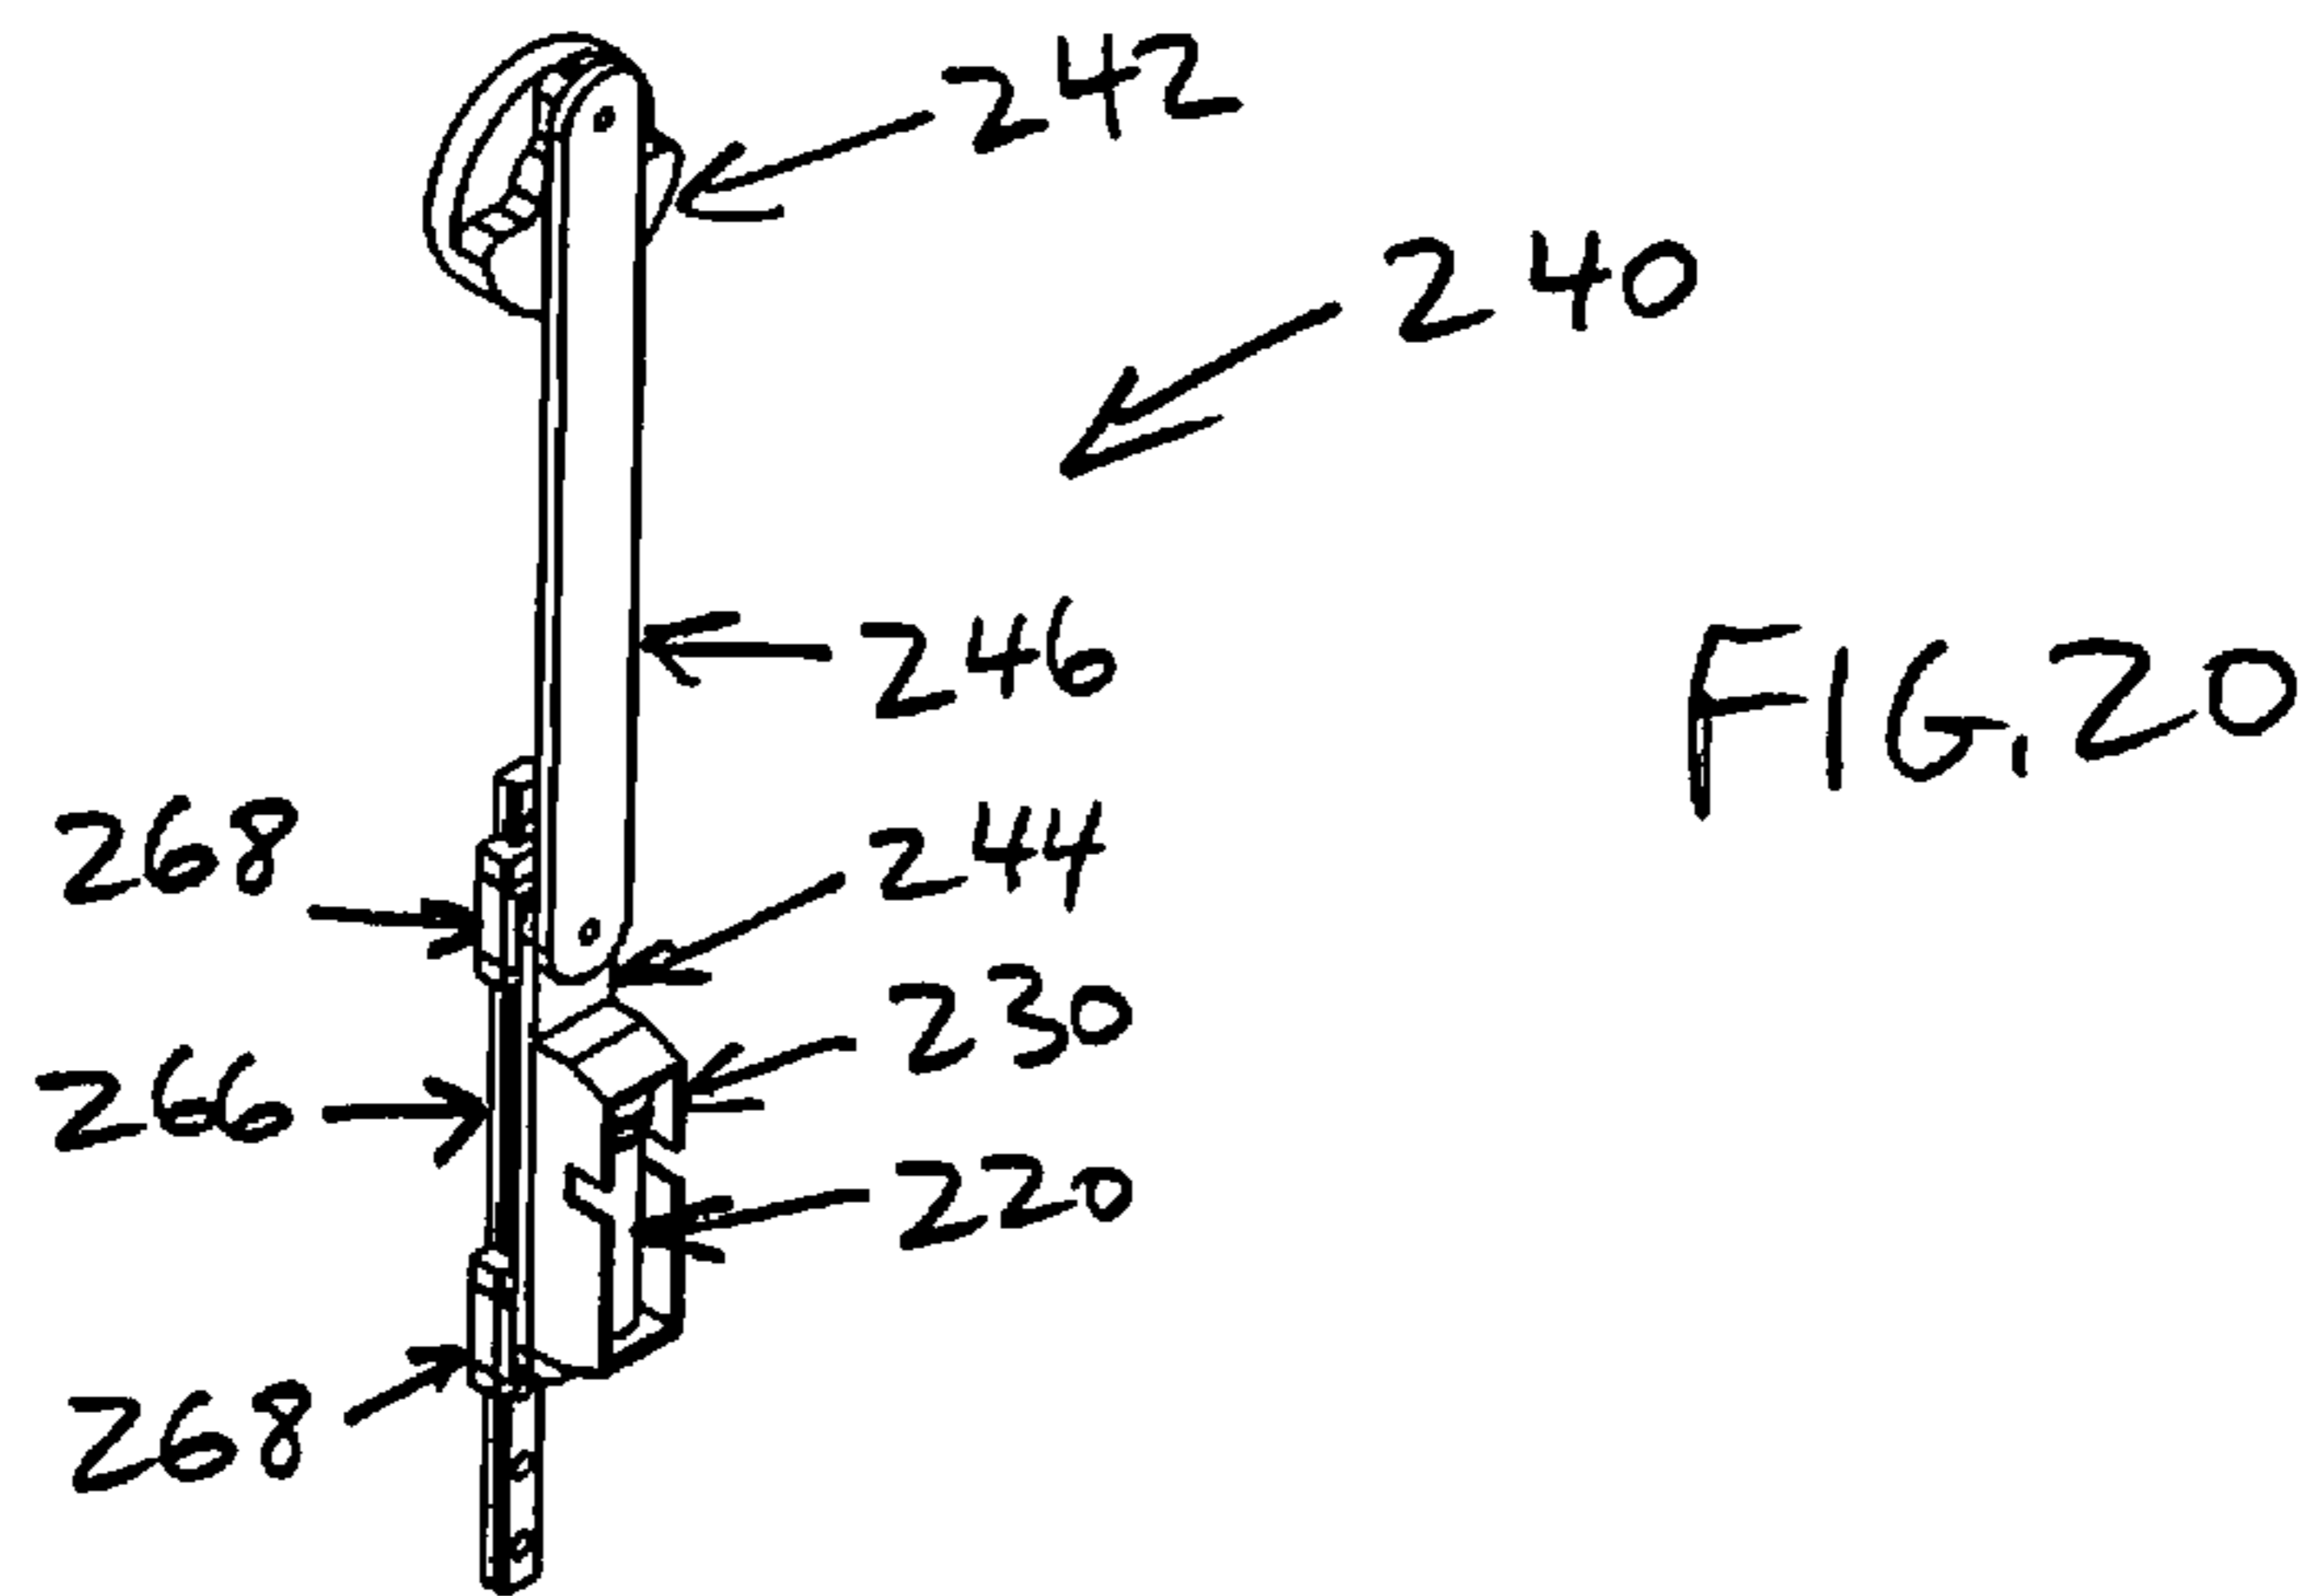

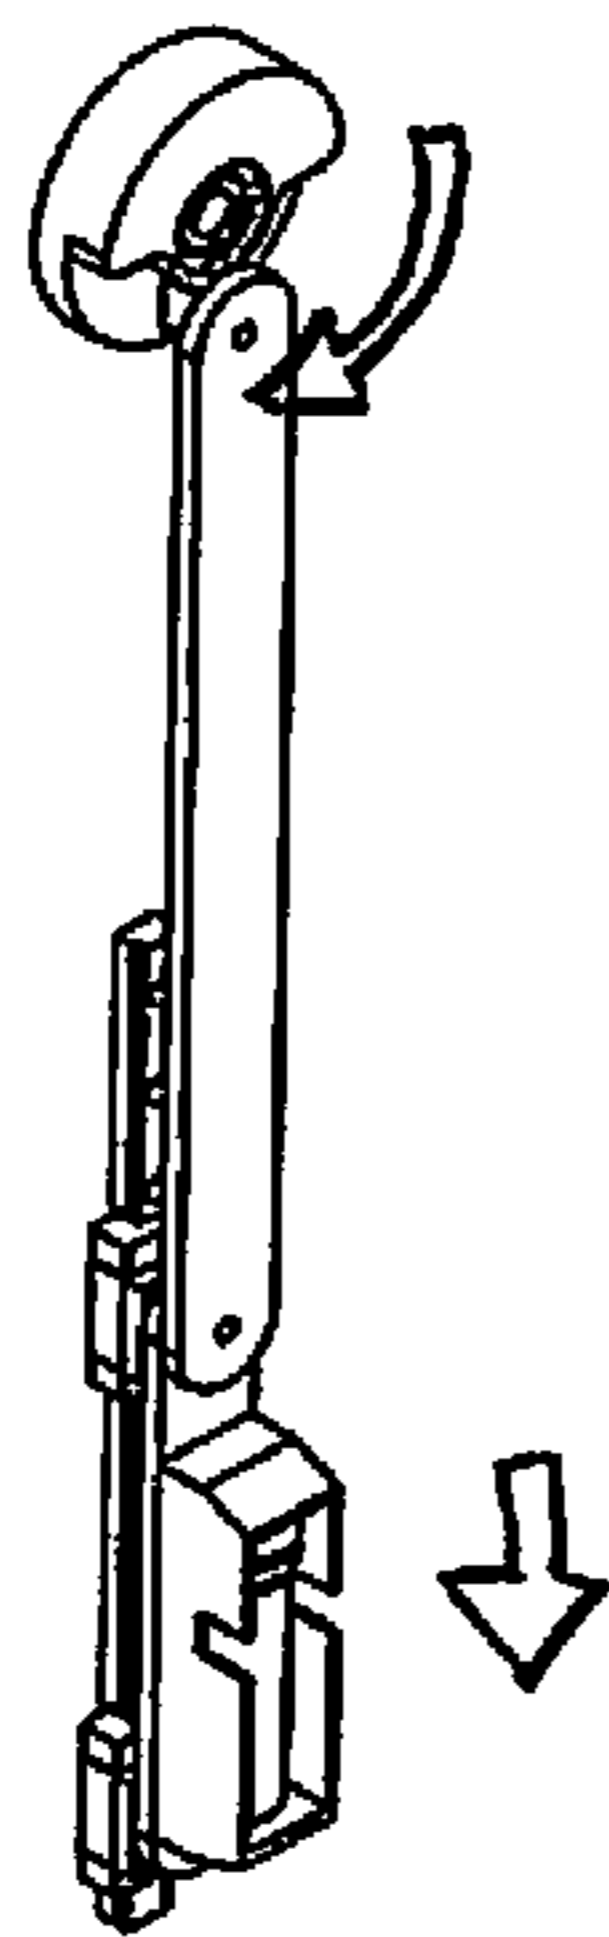


240

FIG. 22

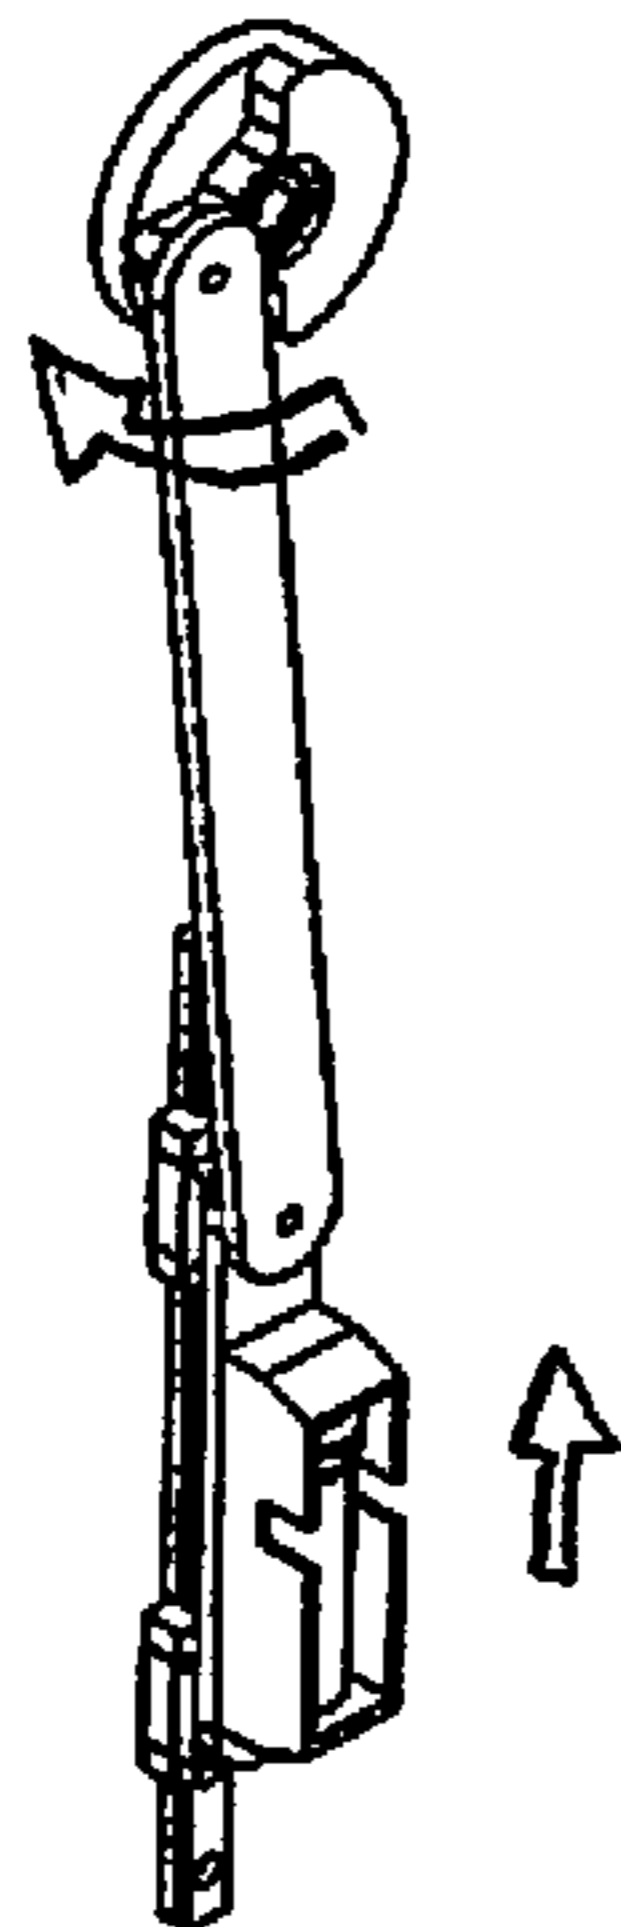


240

FIG. 23

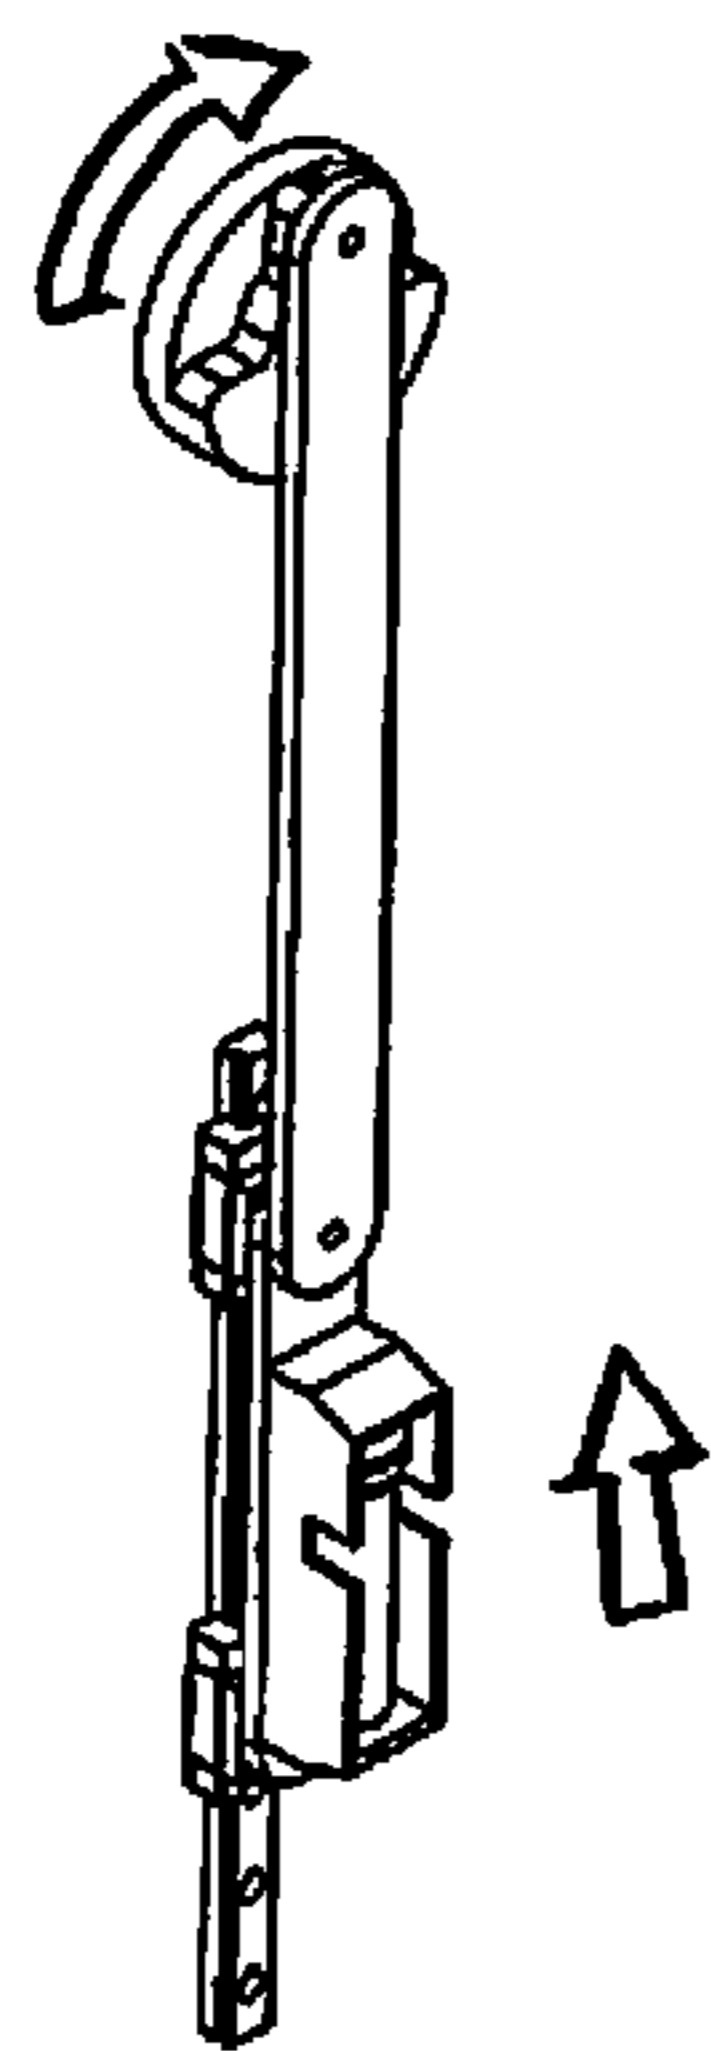

← 240

FIG. 24

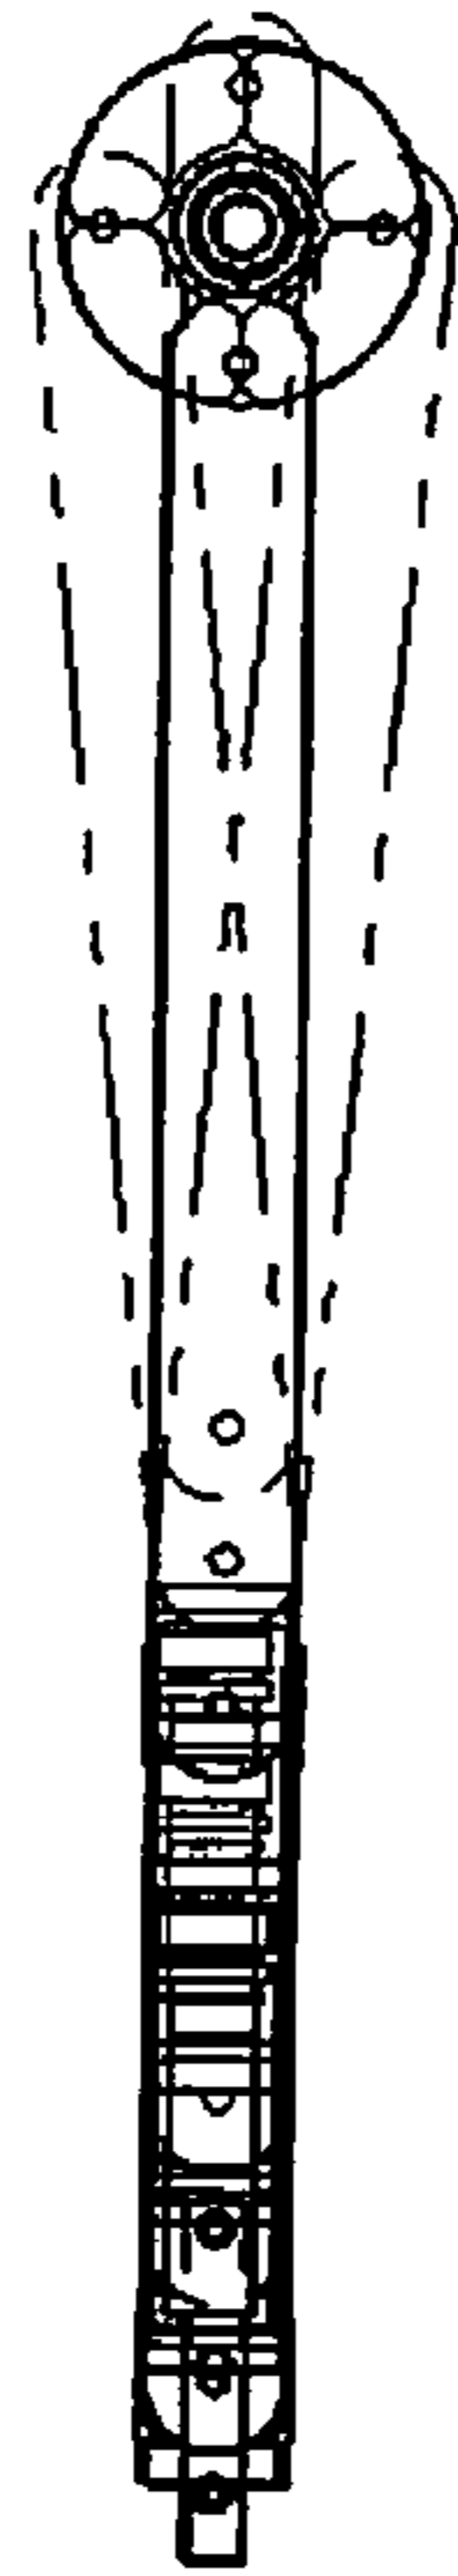

240

FIG. 25



240

FIG. 26

1

RECIPROCATING TUBE-SHAKING MECHANISMS FOR PROCESSING A MATERIAL

CROSS-REFERENCE TO RELATED APPLICATION

This application claims the priority benefit of U.S. Provisional Patent Application Ser. No. 62/072,655, filed Oct. 30, 2014, which is hereby incorporated herein by reference.

TECHNICAL FIELD

The present invention relates generally to laboratory devices for homogenizing sample materials, and particularly to reciprocating mechanisms for inclusion in homogenizing devices to generate reciprocal agitation motions and forces on the samples.

BACKGROUND

Homogenization involves disaggregating or emulsifying the components of a sample using a high-shear process with significant micron-level particle-size reduction of the sample components. Homogenization is commonly used for a number of laboratory applications such as creating emulsions, reducing agglomerate particles to increase reaction area, cell destruction for capture of DNA material (proteins, nucleic acids, and related small molecules), DNA and RNA amplification, and similar activities in which the sample material is bodily tissue and/or fluid, or another substance. Conventional high-powered mechanical-shear homogenization devices for such applications are commercially available in various designs to generate for example vigorous reciprocating, circular, or “swashing” (sinusoidal) oscillating motions and resulting forces. The samples are held in sample tubes that are mounted to tube holders that are mounted to the homogenization device such that the vigorous oscillating forces are transmitted through the tube holders and the tubes to the contained samples.

These homogenization devices have proven generally beneficial in accomplishing the desired homogenization of the sample materials. But in use they have their disadvantages. For example, the linear reciprocating motion tends to produce less of a grinding shear action on the samples and instead merely causes the samples to linearly traverse the lengths of the tubes (with little disaggregation) and smash against the ends of the tubes (with the impacts causing disaggregation). In addition, these impacts tend to create a lot of heat in the tubes, which can degrade the samples to be processed.

Accordingly, it can be seen that needs exist for improvements in reciprocating mechanisms of homogenization devices to provide better homogenization of the sample materials. It is to the provision of solutions to this and other problems that the present invention is primarily directed.

SUMMARY

Generally described, the present invention relates to agitation mechanisms for homogenization devices for processing sample materials in tubes that are secured by tube holders to the agitation mechanisms. Each agitation mechanism includes a first rotary member having a first fixed rotational axis, a second rotary member having a second fixed rotational axis, and a connecting member that extends between them and is rotationally mounted to them at third

2

and fourth non-fixed rotational axes, with the tube holder mounted to the connecting member (or the second rotary member), with the first and third rotational axes defining a first offset, and with the second and fourth rotational axes defining a second offset. When the first rotary member is driven through rotation, the sample in the tube in the tube holder on the connecting member is driven through a nonlinearly reciprocating motion profile to produce a grinding shear action to better homogenize the samples.

In some embodiments, the first and second offsets are different to produce a nonlinearly reciprocating motion profile of a centroid of the tube that is not symmetrical about a transverse axis of the tube. In other embodiments, the first and second offsets are substantially equal to produce a nonlinearly reciprocating motion profile of a centroid of the tube that is symmetrical about a transverse axis of the tube. And in yet other embodiments, the second rotary member is eliminated and replaced with a linear slide carriage to which the tube holder is mounted to produce a linearly reciprocating motion profile of a centroid of the tube.

The specific techniques and structures employed to improve over the drawbacks of the prior devices and accomplish the advantages described herein will become apparent from the following detailed description of example embodiments and the appended drawings and claims.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of an agitation mechanism according to a first example embodiment of the present invention, showing a portion of a homogenization device its incorporated into, a tube holder mounted to it, and a sample-holding tube mounted to the tube holder.

FIG. 2 shows the agitation mechanism of FIG. 1 in use with the crank member in a 12 o'clock position.

FIG. 3 shows the agitation mechanism of FIG. 2 in use with the crank member rotated to a 3 o'clock position.

FIG. 4 shows the agitation mechanism of FIG. 3 in use with the crank member rotated further to a 6 o'clock position.

FIG. 5 shows the agitation mechanism of FIG. 4 in use with the crank member rotated further to a 9 o'clock position.

FIG. 6 shows the agitation mechanism of FIG. 5 in use with the crank member rotated further back to the 12 o'clock position.

FIG. 7 is a side view of the agitation mechanism of FIG. 1, with the four positions of FIGS. 2-6 shown in phantom lines.

FIG. 8 is a perspective view of the agitation mechanism of FIG. 7.

FIG. 9 is a side view of the agitation mechanism of FIG. 1, showing a motion profile traced as a centroid of the tube moves through the four positions of FIG. 7.

FIG. 9A shows the agitation mechanism of FIG. 9 with two alternative locations for the tube centroid for producing two alternative agitation motion profiles.

FIG. 10 is a perspective view of an agitation mechanism according to a second example embodiment of the present invention, showing a tube holder mounted to it and a sample-holding tube mounted to the tube holder.

FIG. 11 shows the agitation mechanism of FIG. 10 in use with the crank member in a 12 o'clock position.

FIG. 12 shows the agitation mechanism of FIG. 11 in use with the crank member rotated to a 3 o'clock position.

3

FIG. 13 shows the agitation mechanism of FIG. 12 in use with the crank member rotated further to a 6 o'clock position.

FIG. 14 shows the agitation mechanism of FIG. 13 in use with the crank member rotated further to a 9 o'clock position.

FIG. 15 shows the agitation mechanism of FIG. 14 in use with the crank member rotated further back to the 12 o'clock position.

FIG. 16 is a side view of the agitation mechanism of FIG. 10, with the four positions of FIGS. 11-15 shown in phantom lines.

FIG. 17 is a perspective view of the agitation mechanism of FIG. 16.

FIG. 18 is a side view of the agitation mechanism of FIG. 10, showing a motion profile traced as a centroid of the tube moves through the four positions of FIG. 16.

FIG. 19 is a perspective view of an agitation mechanism according to a third example embodiment of the present invention, showing a tube holder mounted to it and a sample-holding tube mounted to the tube holder.

FIG. 20 shows the agitation mechanism of FIG. 19 in use with the crank member in a 12 o'clock position.

FIG. 21 shows the agitation mechanism of FIG. 20 in use with the crank member rotated to a 3 o'clock position.

FIG. 22 shows the agitation mechanism of FIG. 21 in use with the crank member rotated further to a 6 o'clock position.

FIG. 23 shows the agitation mechanism of FIG. 22 in use with the crank member rotated further to a 9 o'clock position.

FIG. 24 shows the agitation mechanism of FIG. 23 in use with the crank member rotated further back to the 12 o'clock position.

FIG. 25 is a side view of the agitation mechanism of FIG. 19, with the four positions of FIGS. 20-23 shown in phantom lines.

FIG. 26 is a perspective view of the agitation mechanism of FIG. 25.

DESCRIPTION OF EXAMPLE EMBODIMENTS

The present invention relates primarily to agitation mechanisms of homogenization devices for generating nonlinearly reciprocating motions and resulting forces on tubes mounted to the device and thus to samples contained in the tubes. By the use of the agitation mechanisms, the nonlinearly reciprocating forces on the samples in the tubes tend to cause the samples to move not just back and forth between the ends of the tubes (i.e., along the axial lengths of the tubes) but also somewhat transversely (i.e., laterally) back and forth between the sides of the tubes (i.e., across the widths of the tubes) to produce a grinding shear action to better homogenize the samples and to avoid excess heat generation.

It should be noted that the agitation mechanisms can be used with a wide variety of different types of homogenization devices, tube holders, tubes, and sample materials, and as such these terms as used herein are intended to be broadly construed. Accordingly, the term "homogenizing device" includes shakers, bead mills, vortexers, centrifuges, other sample-agitation devices, and other devices for processing samples by generating and applying vigorous oscillating agitation forces, for laboratory and/or other applications. The term "processing" means particle-size reduction of the sample by use of one or more of the homogenizing devices disclosed herein or known to persons of ordinary skill in the

4

art. The term "tube holder" includes any plate, clamp, clip, cassette, or other retaining structure that can hold one or more sample tubes during homogenization. The term "tube" includes any sealable vessel or container that can hold a sample during homogenization and is not necessarily limited to conventional clear, plastic, cylindrical vials. And the term "sample" includes any type of substance that can be homogenized and for which homogenization could be useful, such as but not limited to human or non-human bodily fluid and/or tissue (e.g., blood, bone-marrow cells, a coronary artery segment, or pieces of organs), other organic matter (e.g., plants or food), and/or other chemicals.

Turning now to the drawings, FIGS. 1-9 show a nonlinearly reciprocating agitation mechanism 40 according to a first example embodiment of the invention. The agitation mechanism 40 can be readily incorporated into a conventional homogenization device 10, as is understood by persons of ordinary skill in the art, to transmit nonlinearly reciprocating motions and resulting forces through a tube holder 30 holding a tube 20 containing a sample material to homogenize the sample. In typical embodiments, the homogenization device 10 includes a drive system (e.g., an electric rotary motor 12) for driving the agitation mechanism 40, an electric power source or connection (e.g., a power cord) for powering the drive system, a control system (e.g., a programmed controller, inputs such as buttons and a keypad, and outputs such as a display screen, for functions such as on/off, start/stop, speed, and time) for operating the drive system, and a housing and/or frame 14 that at least partially encloses and/or supports the agitation mechanism, the drive system, and the control system. These major components of the homogenization device can be of a conventional type well known in the art, so exacting details are not included herein.

The agitation mechanism 40 includes a first rotary member 42, a second rotary member 44, and a connecting member 46 that extends between them and to which the tube holder 30 is mounted. One of the first and second rotary members 42 and 44 is operably coupled to a rotary drive/output shaft 16 of the drive system 12 of the homogenizer 10 at a first fixed rotational axis 50, with this rotary member also referred to as the crank member. And the other one of the first and second rotary members 42 and 44 is rotationally mounted in a fixed location for example by a pin 48 to the housing or frame 14 of the homogenizer 10 at a second fixed rotational axis 52, with this rotary member also referred to as the rocker member. In the depicted embodiment, for example, the first rotary member 42 is the crank member and the second rotary member 44 is the rocker member.

The crank and rocker rotary members 42 and 44 can be provided by various different structures, including wheels (e.g., solid disks or peripheral-frame hoops), wedges (i.e., portions of wheels), link arms (e.g., flat, thin blades), or other conventional rotary structures. And the connecting member 46 can be provided by various different structures, including link arms (e.g., flat, thin blades), rods, bars, plates, panels, or other conventional structures for rotationally connecting two parts. In the depicted embodiment, for example, the crank member 42 is a wheel, the rocker member 44 is a link arm, and the connecting member 46 is a link arm.

The connecting member 46 is rotationally coupled (e.g., by rotation-permitting pins) to the crank and rocker rotary members 42 and 44 at third and fourth non-fixed rotational axes 54 and 56, respectively. The crank and rocker rotary members 42 and 44 have different diameters of rotation. (As used herein, the pivoting motion of the rocker rotary mem-

ber is considered to be rotational because it forms a curve even though not a complete 360-degree curve.) In other words, the third rotational axis **54** is offset from the first rotational axis **50** by a crank offset **58**, and the fourth rotational axis **56** is offset from the second rotational axis **52** by a rocker offset **60**, with the crank and rocker offsets not being equal. The rocker offset **60** is sufficiently longer (e.g., about three times longer in the depicted embodiment) than the crank offset **58** that the third rotational axis **54** curves through a complete 360-degree path around the first rotational axis **50** with a constant angular speed, while the fourth rotational axis **56** sweeps back and forth through an arc (with a longitudinal component and a transverse component) radiused from the second rotational axis **52** with cyclically increasing and decreasing angular speeds, and while the sample in the tube **20** is subjected to cyclically increasing and decreasing angular speeds (and resulting acceleration and deceleration forces) due to mechanically imparted forces due to the transverse motion component (and resulting transverse forces) of the nonlinear reciprocation.

The tube holder **20** can be designed to hold one tube **30** (as depicted) or multiple tubes. The tube holder **20** can be fixedly or removably mounted to the agitation mechanism **10** at a mounting location **11** by conventional mounting structures such as pins, rivets, adhesives, clamps, etc. In the depicted embodiment, the tube holder **20** is mounted at a mounting location **11** on the connecting member **46** to move in a parallel (including the same) plane, and is generally aligned with the third and fourth non-fixed rotational axes **54** and **56**. In other embodiments, the tube holder is mounted at a mounting location on the rocker member to move in a parallel (including the same) plane. Typically, the tube holder **20** includes clamping or other retention structures that grip the tube **30** to releasably hold it in place with a snap fit. The tube holder **20** can be of a conventional type well known in the art, so exacting details are not included herein. In some embodiments, the tube holder is of the type disclosed in U.S. patent application Ser. No. 14/884,989 filed Oct. 16, 2015, which is hereby incorporated herein by reference. In other embodiments, the tube holder and the connecting member (or the second member) are integrally formed as a single piece.

FIGS. 2-6 show the use of the agitation mechanism **40** of the homogenization device **10** to process a sample material in one cycle of reciprocation, with the crank member **42** being driven through a complete 360-degree rotational cycle (as indicated by the upper angular directional arrows) from the 12 o'clock position (FIG. 2), to the 3 o'clock position (FIG. 3), to the 6 o'clock position (FIG. 4), to the 9 o'clock position (FIG. 5), and back to the 12 o'clock position (FIG. 6) to drive the rocker member **44** through its rocking motion (as indicated by the lower angular directional arrows). And FIGS. 7 and 8 each show this same one cycle of reciprocation in one view (so the four positions shown in phantom lines in each of FIGS. 7 and 8 correspond to the four positions of FIGS. 2/6, 3, 4 and 5).

In particular, the control system is operated to rotate the drive shaft **16** of the drive system **12**, which in turn rotates the crank wheel **42** of the agitation mechanism **40**. This rotation is transmitted from the crank wheel **42**, through the connection arm **46**, to the rocker arm **44**. As the crank wheel **42** rotates, the connection arm **46** and rocker arm **44** rotationally pivot back and forth to create the depicted nonlinear, reciprocating, planar motion profile (i.e., traced path of travel) **62** (see FIG. 9) for a centroid (i.e., the geometric center in all three axes) **22** of the tube **20** (i.e., the internal sample-containing chamber) in the tube holder **30**.

The motion profile **62** of the tube centroid **22** is generally oval or teardrop-shaped, with the upper portion of the motion profile being (relatively slightly) more elliptical/circular/bulbous than the lower portion, which is (relatively slightly) more linear/narrow than the upper portion (so a motion profile of the tube top centroid is more elliptical than a motion profile of the tube bottom centroid, which is more linear than the tube top centroid motion profile). Thus, the motion profile **62** is substantially symmetrical about the longitudinal axis of the tube (including the right side of the depicted motion profile being slightly flatter with the left side being slightly rounder, relatively speaking) but not substantially symmetrical about the transverse axis of the tube **20**. (The motion profile **62** is substantially but not perfectly symmetrical about the vertical/longitudinal axis because the rocker arm **44** pivots back and forth through a slight arc radiused about the rotational axis **52** of the rocker arm, so the motion profile is slightly rounder on the left side and slightly flatter on the right side.) The crank wheel **42** and the rocker arm **44** propel the connection arm **46** in a plane perpendicular to the rotational axes **50** and **52** of the crank wheel and the rocker arm, and as such the sample tube **20** is always parallel to that perpendicular plane. As such, the agitation mechanism **40** advantageously uses a planar quadrilateral linkage system with four rotating joints **50**, **52**, **54**, and **56** to define this unique motion profile **62** with a non-linear path of reciprocating motion that provides for improved grinding characteristics and increased acceleration forces for more-effective processing.

It should be noted that the tube holder **30**, and thus the tube **20** and its centroid **22**, can be located at other positions on the connecting arm **46** to produce different agitation motion profiles. For example, with the tube holder and the tube (and thus the tube centroid) positioned closer to the crank wheel, the corresponding motion profile produced is less elliptical (less vertically/longitudinally elongated, relatively speaking) and more circular, and with them positioned closer to the rocker arm, the corresponding motion profile produced is more elliptical and less circular. In particular, with the tube holder and the tube positioned closer to the crank wheel to define alternative tube centroid **22a** shown in FIG. 9A, the corresponding alternative motion profile **22a** produced is generally circular (and thus transversely wider), and with them positioned closer to the rocker arm to define alternative tube centroid **22b**, the corresponding alternative motion profile **22b** produced is transversely narrower, while the length (vertical/longitudinal dimension) of the motion profiles is the same. (Because the rocker arm **44** pivots back and forth through a slight arc, the motion profiles **22** and **22a** are rounder on the left side and flatter on the right side, with this being more exaggerated the closer the respective tube centroid **62** and **62** is to the rocker arm.) As such, the tube holder can be selectively located to generate a particular agitation motion profile as may be desired for a given application, for example to vary the amount of transverse motion of the tube centroid while keeping the amplitude in the tube axis/longitudinal direction the same.

FIGS. 10-18 show a nonlinearly reciprocating agitation mechanism **140** according to a second example embodiment of the invention. The agitation mechanism **140** is similar to that of the first embodiment, for example it can be readily incorporated into a conventional homogenization device (not shown), as is understood by persons of ordinary skill in the art, to transmit nonlinearly reciprocating motions and resulting forces through a tube holder **130** holding a tube **120** containing a sample material to homogenize the sample. In particular, the agitation mechanism **140** includes a first

rotary member **142** with a first fixed rotational axis **150**, a second rotary member **144** with a second fixed rotational axis **152**, and a connecting member **146** that extends between them, that is rotationally coupled to the first and second rotary members (for example by a rotation-permitting pins) at third and fourth non-fixed rotational axes **154** and **156**, respectively, and to which the tube holder **130** can be mounted.

In this embodiment, however, the first and second rotary members **142** and **144** have the same diameters of rotation. In other words, the third rotational axis **154** is offset from the first rotational axis **150** by the first offset **158**, and the fourth rotational axis **156** is offset from the second rotational axis **152** by the second offset **160**, with the first and second offsets being substantially equal. In this way, the third and fourth rotational axes **154** and **156** curve through a complete 360-degree path around the first and second rotational axes **150** and **152**, respectively, with a constant angular speed, while the sample in the tube **120** is subjected to cyclically increasing and decreasing angular speeds (and resulting acceleration and deceleration forces) due to mechanically imparted forces during the vertical-component reciprocation (i.e., an acceleration force with a constant magnitude in a alternating/changing direction).

In addition, in this embodiment the first rotary member **142** is a crank wheel, the second rotary member **144** is an idler wheel, and the agitation system **140** includes a synchronization loop element (e.g., a belt or chain) **164** that is routed around the crank and idler wheels to coordinate their angular motion.

FIGS. **11-15** show the use of the agitation mechanism **140** of the homogenization device to process a sample material in one cycle of reciprocation, with the crank member **142** being driven through a complete 360-degree rotational cycle (as indicated by the upper angular directional arrows) from the 12 o'clock position (FIG. **11**), to the 3 o'clock position (FIG. **12**), to the 6 o'clock position (FIG. **13**), to the 9 o'clock position (FIG. **14**), and back to the 12 o'clock position (FIG. **15**) to drive the idler member **144** through its rotational motion (as indicated by the lower angular directional arrows). And FIGS. **16** and **17** each show this same one cycle of reciprocation in one view (so the four positions shown in phantom lines in each of FIGS. **16** and **17** correspond to the four positions of FIGS. **11/15**, **12**, **13** and **14**).

In particular, the control system is operated to rotate the drive shaft of the drive system, which in turn rotates the crank wheel **142** of the agitation mechanism **140**. This rotation is transmitted from the crank wheel **142** to the idler wheel **144** through the connection arm linkage **146** as well as through the synchronization loop **164**. The synchronized motion of the crank and idler wheels **142** and **144** propels the connection arm linkage **146** in such a way that the sample tube **120** is always parallel to a plane perpendicular to the rotational axes **150** and **152** of the crank and idler wheels. As the crank and idler wheels **142** and **144** rotate, the connection arm linkage **146** rotates in a circle to create the depicted nonlinear, reciprocating, planar motion profile **162** (see FIG. **18**) for a centroid **122** (and top and bottom) of the tube **120** in the tube holder **130**. As a result, the motion profile **162** of the tube centroid **122** is substantially circular, and thus symmetrical about the longitudinal and transverse axes of the tube **120**. As such, the agitation mechanism **140** advantageously uses a planar quadrilateral linkage system with four rotating joints **150**, **152**, **154**, and **156** to define this unique motion profile **162** with a non-linear path of motion

that provides for improved grinding characteristics and increased acceleration forces for more-effective processing.

FIGS. **19-26** show a linearly reciprocating agitation mechanism **240** according to a third example embodiment of the invention. The agitation mechanism **240** has some similarities to that of the first embodiment, for example it can be readily incorporated into a conventional homogenization device (not shown), as is understood by persons of ordinary skill in the art, to transmit reciprocating motions and resulting forces through a tube holder **230** holding a tube **220** containing a sample material to homogenize the sample. In particular, the agitation mechanism **240** includes a first rotary member **242** with a fixed rotational axis **250**, and a connecting member **246** that is rotationally coupled to the first rotary member at a non-fixed rotational axis **254** to define an offset **258** for using rotational motion to guide the tube holder **230** through a reciprocating processing motion.

In this embodiment, however, the second member **244** linearly reciprocates to guide the tube holder **230** and thus the tube **220** through a linearly reciprocating motion profile **262**. As such, this embodiment does not provide the advantages of the nonlinear, reciprocating, planar motion profiles described above, and instead represents an improved agitation mechanism that converts a rotational drive motion to a linear reciprocating processing motion. In particular, the second member **244** is a slide carriage that is rotationally coupled to the connecting member **246** (for example by a rotation-permitting pin) at a non-fixed rotational axis **256** and that linearly reciprocates along a linear slide guide **266** and is linearly guided by one or more sliders **268**. For example, in the depicted embodiment the slide guide **266** is in the form of a male member (e.g., a rail) and there are two sliders **268** in the form of female members (e.g., slide receivers) that slidingly receive the male rail member. In other embodiments, these slide guide is a female member and the slider is a male member slidingly received in the female member. And the tube holder **230** is fixedly mounted to and moves with the slide carriage **244**.

FIGS. **20-24** show the use of the agitation mechanism **240** of the homogenization device to process a sample material in one cycle of reciprocation, with the crank member **242** being driven through a complete 360-degree rotational cycle (as indicated by the upper angular directional arrows) from the 12 o'clock position (FIG. **20**), to the 3 o'clock position (FIG. **21**), to the 6 o'clock position (FIG. **22**), to the 9 o'clock position (FIG. **23**), and back to the 12 o'clock position (FIG. **24**) to drive the slide carriage **244** through its translational motion (as indicated by the lower angular directional arrows). And FIGS. **25** and **26** each show this same one cycle of reciprocation in one view (so the four positions shown in phantom lines in each of FIGS. **25** and **26** correspond to the four positions of FIGS. **20/24**, **21**, **22** and **23**).

In particular, the control system is operated to rotate the drive shaft of the drive system, which in turn rotates the crank wheel **242** of the agitation mechanism **240**. The slide carriage **244** being rotationally mounted to the slider unit(s) **268**, which slidingly engage the linear slide guide component **266**, converts this rotation to a linear reciprocating (e.g., up-and-down) motion of the slide carriage (and thus the attached sample tube **220**) parallel to the linear slide guide and between two travel end-points. Thus, when the crank wheel **242** rotates, the slide carriage **244** slides in a line to create the depicted linear, reciprocating, planar motion profile for a centroid (and top and bottom) of the tube **220** in the tube holder **230**. As such, the agitation mechanism **240** advantageously uses a piston-like mechanism to create

a purely linear motion profile that creates impact forces for more-effective processing with less grinding.

In another embodiment (not shown), a linearly reciprocating agitation mechanism is similar to that of the third example embodiment disclosed herein, except that the slide carriage and the connecting member are combined into a single part. As such, the slide carriage can be considered to be eliminated in this embodiment, with the tube holder mounted to the connecting member (just not immediately adjacent the crank member) and with the connecting member slidingly mounted to the linear slide guide by one or more sliders.

In yet another embodiment (not shown), a nonlinearly reciprocating agitation mechanism is similar to that of the third example embodiment disclosed herein, except that the slide carriage is slidingly mounted to the linear slide guide so that the carriage reciprocates along the slide guide but is not limited to linear motion. For example, the slide carriage can be slidingly mounted to the slide guide by being rotationally coupled to a single slider that is positioned at a lower portion of the carriage (e.g., its bottom end) to permit rotational motion between the carriage and the slider. And the slide carriage can be rotationally coupled to the connection arm at an upper portion of the carriage (e.g., at its top end) to permit rotational motion between the carriage and the connecting arm. So the lower portion of the carriage (at the rotational mount to the linearly guided slider) linearly reciprocates and the upper portion of the carriage (at the rotational mount to the rotationally driven connecting member) is free to rock laterally in a side-to-side manner. As such, this embodiment provides the advantages of the nonlinear, reciprocating, planar (e.g., teardrop/egg-shaped) motion profile described above.

It is to be understood that this invention is not limited to the specific devices, methods, conditions, or parameters described and/or shown herein, and that the terminology used herein is for the purpose of describing particular embodiments by way of example only. Thus, the terminology is intended to be broadly construed and is not intended to be limiting of the claimed invention. For example, as used in the specification including the appended claims, the singular forms “a,” “an,” and “one” include the plural, the term “or” means “and/or,” and reference to a particular numerical value includes at least that particular value, unless the context clearly dictates otherwise. In addition, any methods described herein are not intended to be limited to the sequence of steps described but can be carried out in other sequences, unless expressly stated otherwise herein.

While the invention has been shown and described in exemplary forms, it will be apparent to those skilled in the art that many modifications, additions, and deletions can be made therein without departing from the spirit and scope of the invention as defined by the following claims.

What is claimed is:

1. An agitation mechanism for a laboratory homogenization device for homogenizing a sample in a laboratory tube removably secured in place by a laboratory tube holder, comprising:

a first rotary member having a first fixed rotational axis about which it rotates;

a second rotary member having a second fixed rotational axis about which it rotates;

a connecting member that extends between the first and second rotary members and that is rotationally mounted to the first and second rotary members at respective third and fourth non-fixed rotational axes; and

a mounting location where the laboratory tube holder is positioned,

wherein the first and third rotational axes define a first radial offset and the second and fourth rotational axes define a second radial offset to cooperatively produce a nonlinearly reciprocating motion profile for a centroid of the laboratory tube in the laboratory tube holder, and wherein the nonlinearly reciprocating motion profile produces nonlinearly reciprocating forces on the sample in the laboratory tube that cause the sample to reciprocating move not just longitudinally along lengths of the laboratory tube but also transversely between sides of the laboratory tube to produce a grinding shear action to homogenize the sample, and wherein the first offset is smaller than the second offset so that the third rotational axis of the first rotary member travels through a complete 360-degree path around the first rotational axis, and in response thereto the fourth rotational axis sweeps in a nonlinear reciprocating motion through an arc that is radiused from the second rotational axis, wherein the tube-centroid motion profile is not symmetrical about an axis transverse to a longitudinal axis of the tube and instead is generally oval or teardrop-shaped.

2. The agitation mechanism of claim 1, wherein the third rotational axis of the first rotary member travels through the complete 360-degree path around the first rotational axis with a constant angular speed, and in response thereto the fourth rotational axis sweeps in the nonlinear reciprocating motion through the arc radiused from the second rotational axis at cyclically increasing and decreasing angular speeds.

3. The agitation mechanism of claim 1, wherein the first rotary member is a crank wheel and the second rotary member is a rocker link arm.

4. The agitation mechanism of claim 1, wherein the tube-holder mounting location is on the connecting member so that the laboratory tube holder moves along with the connecting member.

5. The agitation mechanism of claim 4, wherein the laboratory tube holder holds the tube in a parallel plane to the connecting member so that the tube-centroid motion profile is planar.

6. The agitation mechanism of claim 1, wherein the laboratory homogenization device includes a drive system with a drive shaft, and wherein the first rotary member is operably coupled to and driven by the drive shaft.

7. An agitation mechanism for a laboratory homogenization device for homogenizing a sample in a laboratory tube removably secured in place by a laboratory tube holder, comprising:

a first rotary member having a first fixed rotational axis about which it rotates, wherein the first rotary member is a crank wheel, and wherein the first rotary member is operably coupled to and driven by a drive shaft of the laboratory homogenization device;

a second rotary member having a second fixed rotational axis about which it rotates, wherein the second rotational axis is defined by a pin mounted to the laboratory homogenization device;

a connecting member that extends between the first and second rotary members and that is rotationally mounted to the first and second rotary members at respective third and fourth non-fixed rotational axes; and

a mounting location where the laboratory tube holder is positioned, wherein the tube-holder mounting location is on the connecting member so that the laboratory tube holder moves along with the connecting member, wherein the first and third rotational axes define a first radial offset and the second and fourth rotational axes define a

11

second radial offset to cooperatively produce a nonlinearly reciprocating motion profile for a centroid of the laboratory tube in the laboratory tube holder, wherein the first offset and the second offset are not equal so that the tube-centroid motion profile is not symmetrical about an axis transverse to a longitudinal axis of the laboratory tube, wherein the laboratory tube holder holds the laboratory tube in a parallel plane to the connecting member so that the tube-centroid motion profile is planar, and wherein the nonlinearly reciprocating motion profile produces nonlinearly reciprocating forces on the sample in the laboratory tube that cause the sample to reciprocatingly move not just longitudinally along lengths of the laboratory tube but also transversely between sides of the laboratory tube to produce a grinding shear action to homogenize the sample, and wherein the first offset is smaller than the second offset so that the third rotational axis of the first rotary member travels through a complete 360-degree path around the first rotational axis with a constant angular speed, and in response thereto the fourth rotational axis sweeps in a nonlinear reciprocating motion through an arc that is radiused from the second rotational axis and at cyclically increasing and decreasing angular speeds, wherein the tube-centroid motion profile is generally oval or teardrop-shaped.

8. The agitation mechanism of claim 1, wherein the laboratory homogenization device includes a drive system with a drive shaft, and wherein the first rotary member is operably coupled to and driven by the drive shaft.

9. A laboratory homogenization device for homogenizing a sample in a laboratory tube, the laboratory homogenization device comprising:

a drive system including with a drive shaft and a motor that drives the drive shaft; and

an agitation mechanism for processing the sample in the laboratory tube, the agitation mechanism comprising:

a first rotary member having a first fixed rotational axis about which it rotates, wherein the first rotary member is operably coupled to and rotationally driven about the first fixed rotational axis by the drive shaft;

a second rotary member having a second fixed rotational axis about which it rotates, wherein the second rotational axis is defined by a pivotal mount to the laboratory homogenization device;

12

a connecting member that extends between the first and second rotary members and that is rotationally mounted to the first and second rotary members at respective third and fourth non-fixed rotational axes; and

a laboratory tube holder that removably secures the laboratory tube in place, wherein the tube holder is positioned on the connecting member so that the tube holder moves along with the connecting member, wherein the tube holder holds the laboratory tube in a parallel plane to the connecting member so that a motion profile of a centroid of the laboratory tube in the tube holder is planar,

wherein the first and third rotational axes define a first radial offset and the second and fourth rotational axes define a second radial offset, wherein the first offset is smaller than the second offset so that the third rotational axis of the first rotary member travels through a complete 360-degree path around the first rotational axis, and in response thereto the fourth rotational axis sweeps in a nonlinear reciprocating motion through an arc that is radiused from the second rotational axis, wherein the tube-centroid motion profile is nonlinearly reciprocating, non-symmetrical about an axis transverse to a longitudinal axis of the tube, and generally oval or teardrop-shaped, and wherein the nonlinearly reciprocating motion profile produces nonlinearly reciprocating forces on the sample in the laboratory tube that cause the sample to reciprocatingly move not just longitudinally along lengths of the laboratory tube but also transversely between sides of the laboratory tube to produce a grinding shear action to homogenize the samples.

10. The laboratory homogenization device of claim 9, wherein the third rotational axis of the first rotary member travels through the complete 360-degree path around the first rotational axis with a constant angular speed, and in response thereto the fourth rotational axis sweeps in the nonlinear reciprocating motion through the arc radiused from the second rotational axis at cyclically increasing and decreasing angular speeds.

11. The laboratory homogenization device of claim 9, wherein the first rotary member is a crank wheel and the second rotary member is a rocker link arm.

* * * * *