

US010238509B2

(12) **United States Patent**  
**Penenberg**

(10) **Patent No.:** **US 10,238,509 B2**  
(45) **Date of Patent:** **Mar. 26, 2019**

(54) **TELESCOPIC GUIDE FOR HIP REPLACEMENT METHOD**

(71) Applicant: **Crescent H Trust**, Jackson, WY (US)

(72) Inventor: **Brad L. Penenberg**, Los Angeles, CA (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 254 days.

(21) Appl. No.: **14/723,413**

(22) Filed: **May 27, 2015**

(65) **Prior Publication Data**  
US 2015/0250619 A1 Sep. 10, 2015

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 13/623,073, filed on Sep. 19, 2012, now Pat. No. 9,308,003, which  
(Continued)

(51) **Int. Cl.**  
*A61F 2/46* (2006.01)  
*A61B 34/10* (2016.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... *A61F 2/4657* (2013.01); *A61B 17/00234* (2013.01); *A61B 17/164* (2013.01); *A61B 17/1659* (2013.01); *A61B 17/1666* (2013.01); *A61B 17/1668* (2013.01); *A61B 34/10* (2016.02); *A61B 90/11* (2016.02); *A61F 2/34* (2013.01); *A61F 2/4609* (2013.01); *A61B 2017/00075* (2013.01); *A61B 2017/3405* (2013.01); *A61B 2017/922* (2013.01); *A61B 2034/107* (2016.02); *A61B 2034/2048* (2016.02); *A61B 2034/2055* (2016.02);  
(Continued)

(58) **Field of Classification Search**

CPC .. *A61F 2/4657*; *A61F 2/4609*; *A61B 17/1746*; *A61B 17/1742*; *B25H 7/00*

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,808,185 A 2/1989 Penenberg  
4,813,149 A \* 3/1989 Herkimer ..... B25H 7/00  
33/451

(Continued)

FOREIGN PATENT DOCUMENTS


WO WO 2010/030809 3/2010  
WO WO 2010/031111 3/2010

*Primary Examiner* — Andrew Yang

(57) **ABSTRACT**

A tool for locating a proper position for a portal incision for hip arthroplasty, the tool having at least one generally elongated body defining an axis, the generally elongated body having a slot at one end, the slot being angled at an approximately 45 degree angle relative to the axis of the generally elongated body, the slot configured to receive a cutting member or guide tool. A second generally elongated body may be connected to the first generally elongated body to form a right angle. If the lengths of the two generally elongated bodies are substantially equivalent, then when the second generally elongated body is inserted into the acetabulum, the first generally elongated body positions the slot in the proper location such that sliding a guide tool or cutting member through the slot allows a portal incision to be created in the proper location. In some embodiments, the generally elongated bodies may have adjustable lengths.

**15 Claims, 17 Drawing Sheets**

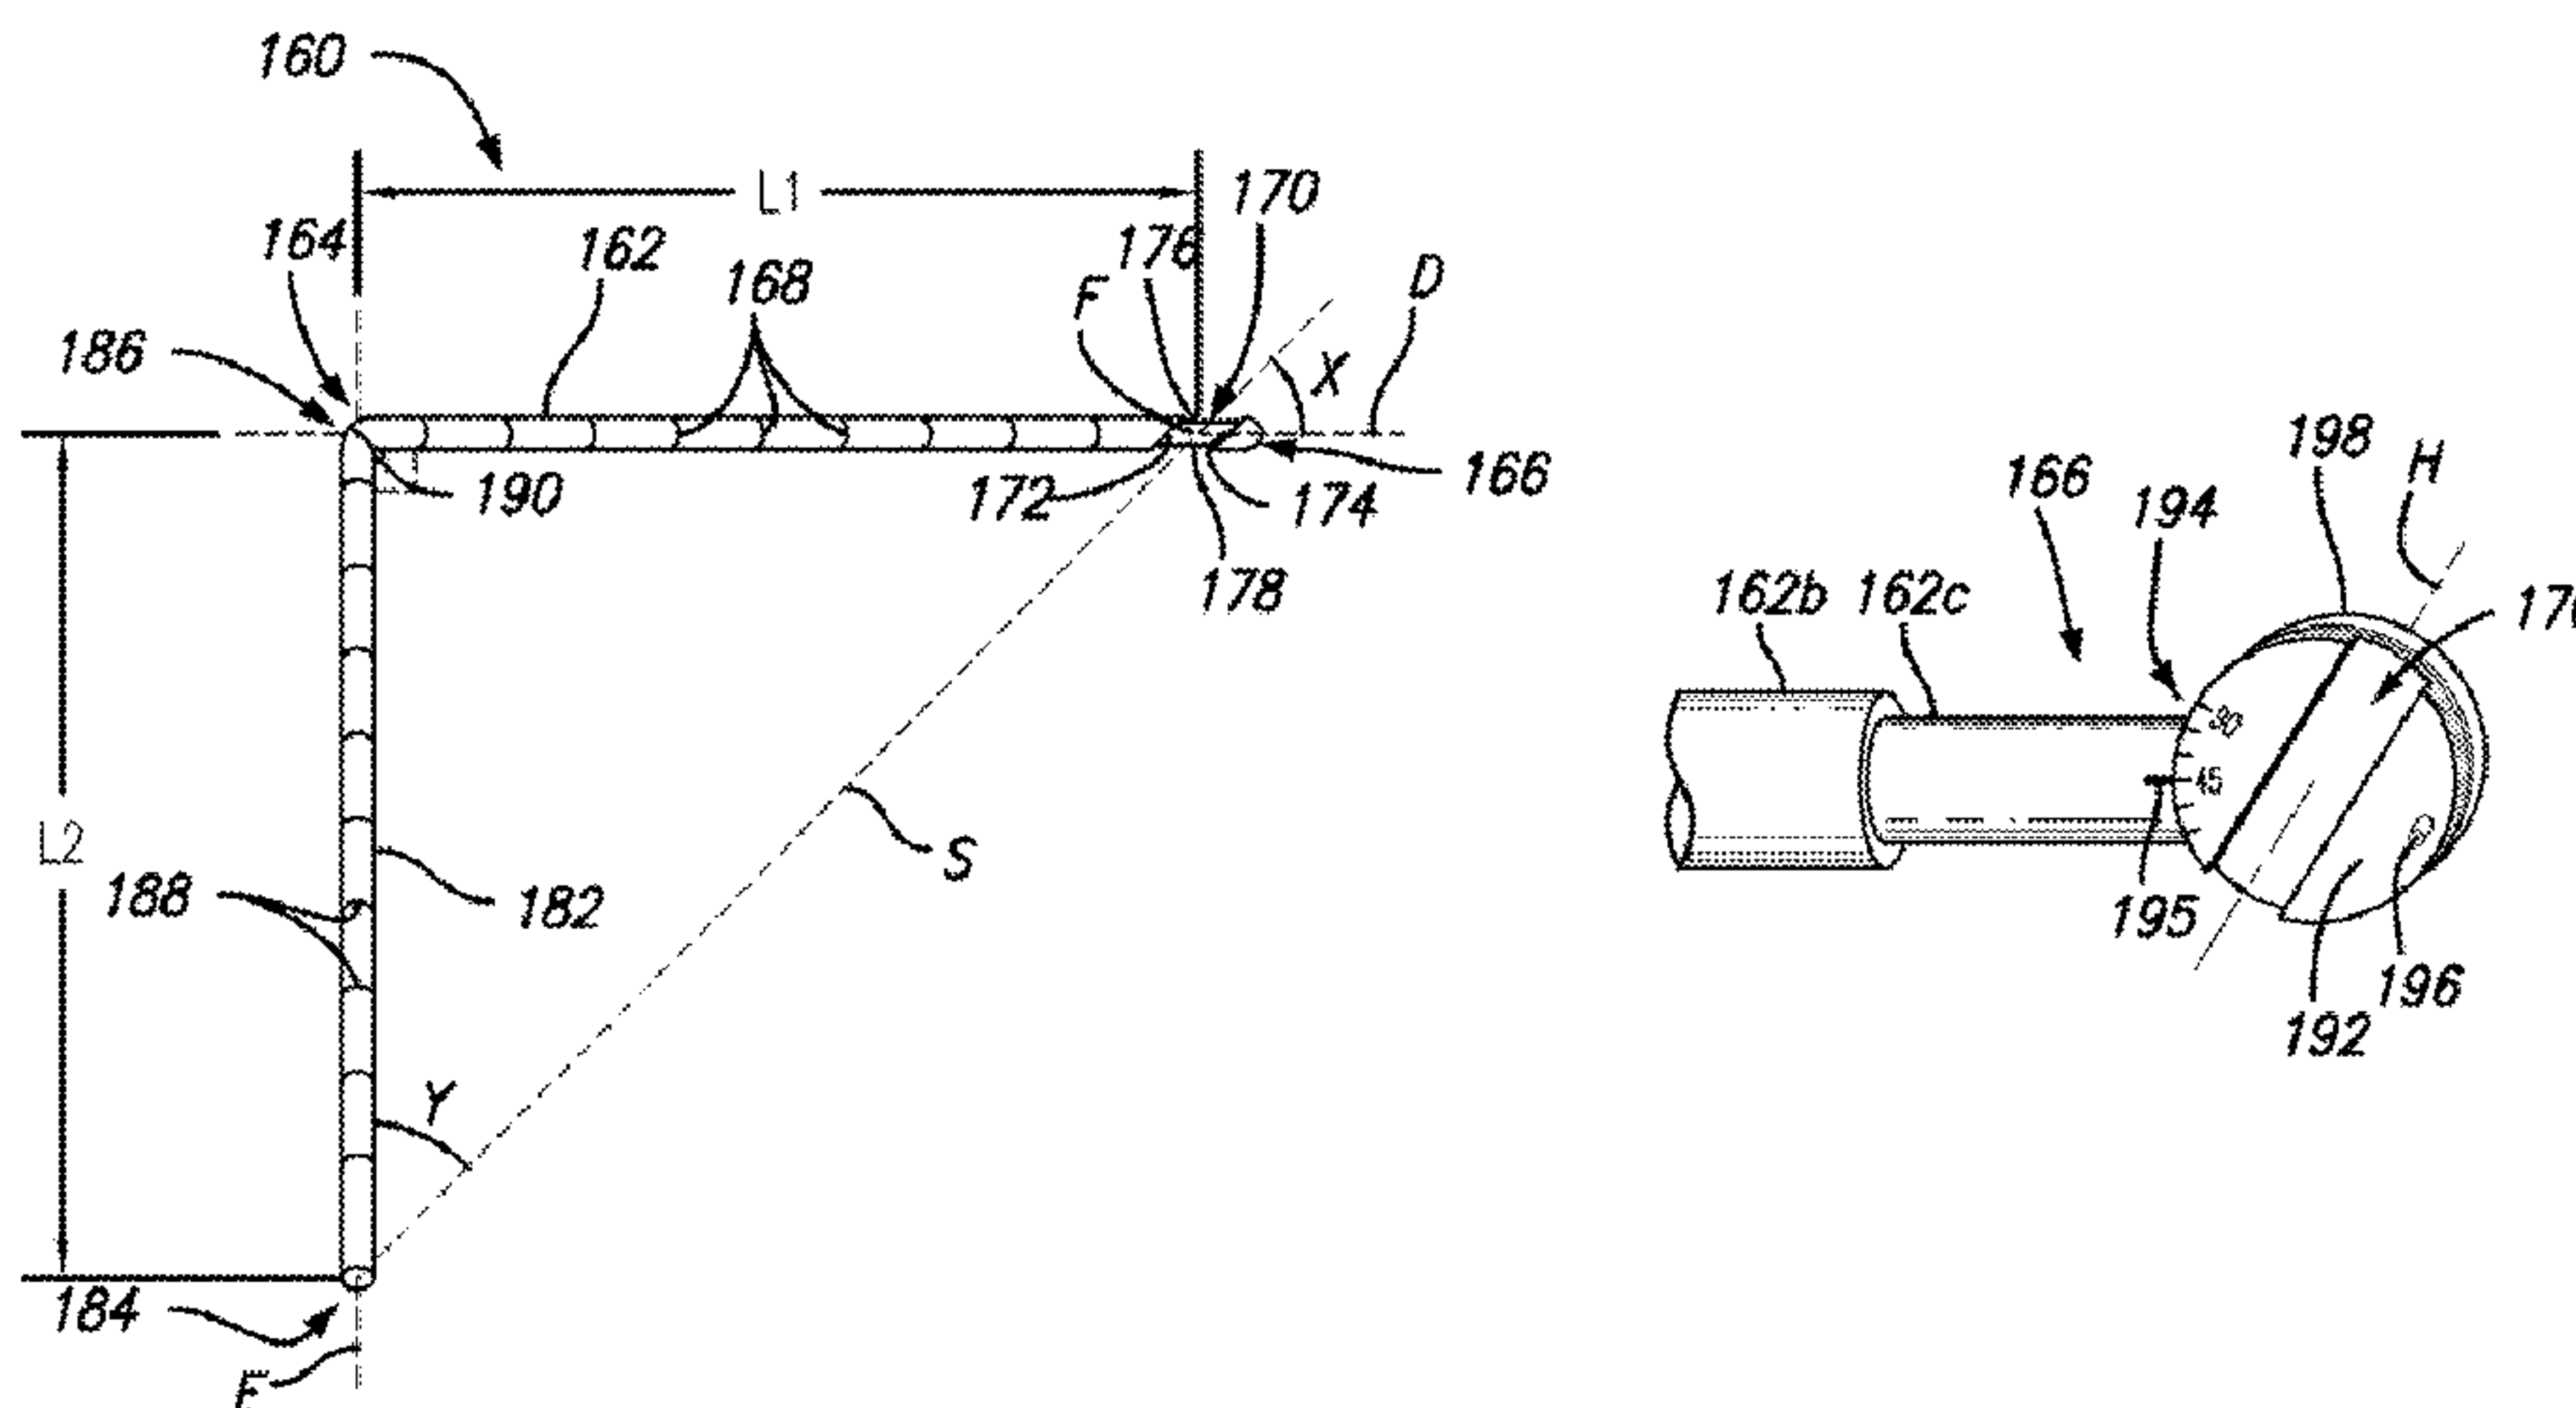

**Related U.S. Application Data**

is a continuation of application No. 13/440,962, filed on Apr. 5, 2012, now Pat. No. 9,439,675, which is a continuation of application No. 13/431,944, filed on Mar. 27, 2012, now Pat. No. 9,610,092.

(60)	Provisional application No. 61/528,744, filed on Aug. 29, 2011, provisional application No. 61/567,869, filed on Dec. 7, 2011.	5,989,259 A	11/1999	Penenberg	
		6,589,285 B2	7/2003	Penenberg	
		6,697,664 B2	2/2004	Kienzle, III et al.	
		6,905,502 B2	6/2005	Penenberg	
		6,997,928 B1	2/2006	Penenberg	
		D553,751 S	10/2007	Penenberg	
		7,396,328 B2	7/2008	Penenberg	
		7,582,090 B2	9/2009	Penenberg	
		7,651,501 B2	1/2010	Penenberg	
		7,660,624 B2	2/2010	Georg et al.	
		7,702,379 B2	4/2010	Avinash et al.	
(51)	<b>Int. Cl.</b>	7,819,879 B2	10/2010	Penenberg	
	<i>A61B 17/16</i> (2006.01)	7,833,229 B2	11/2010	Penenberg	
	<i>A61B 90/11</i> (2016.01)	7,931,657 B2*	4/2011	Walters .....	A61B 17/1725 606/98
	<i>A61B 17/00</i> (2006.01)				
	<i>A61F 2/34</i> (2006.01)	8,034,057 B2	10/2011	Penenberg	
	<i>A61B 90/00</i> (2016.01)	8,439,928 B2	5/2013	Penenberg	
	<i>A61B 17/34</i> (2006.01)	8,740,907 B2	6/2014	Penenberg	
	<i>A61F 2/30</i> (2006.01)	8,831,324 B2	9/2014	Penenberg	
	<i>A61B 34/20</i> (2016.01)	2003/0229352 A1	12/2003	Penenberg	
	<i>A61B 17/92</i> (2006.01)	2004/0181149 A1	9/2004	Langlotz et al.	
(52)	<b>U.S. Cl.</b>	2005/0149050 A1	7/2005	Stifter et al.	
	CPC ... <i>A61B 2090/061</i> (2016.02); <i>A61B 2090/067</i> (2016.02); <i>A61B 2090/0811</i> (2016.02); <i>A61F 2002/3055</i> (2013.01); <i>A61F 2002/30471</i> (2013.01); <i>A61F 2002/30553</i> (2013.01); <i>A61F 2002/30601</i> (2013.01); <i>A61F 2002/4623</i> (2013.01); <i>A61F 2002/4668</i> (2013.01); <i>A61F 2002/4681</i> (2013.01); <i>A61F 2002/4687</i> (2013.01)	2006/0217737 A1	9/2006	Iverson	
		2009/0099570 A1	4/2009	Paradis et al.	
		2009/0099665 A1	4/2009	Taylor et al.	
		2009/0138019 A1	5/2009	Wasielewski	
		2010/0076505 A1	3/2010	Borja	
		2011/0015642 A1	1/2011	Penenberg	
		2012/0116412 A1	5/2012	Penenberg	
		2013/0053856 A1	2/2013	Penenberg	
		2013/0053857 A1	2/2013	Penenberg	
		2013/0053858 A1	2/2013	Penenberg	
		2013/0053859 A1	2/2013	Penenberg	
(56)	<b>References Cited</b>	2013/0053904 A1	2/2013	Penenberg	
	<b>U.S. PATENT DOCUMENTS</b>	2013/0190770 A1	7/2013	Penenberg	
	5,788,705 A	8/1998		Huddleston et al.	
	5,910,172 A	6/1999		Penenberg	

\* cited by examiner

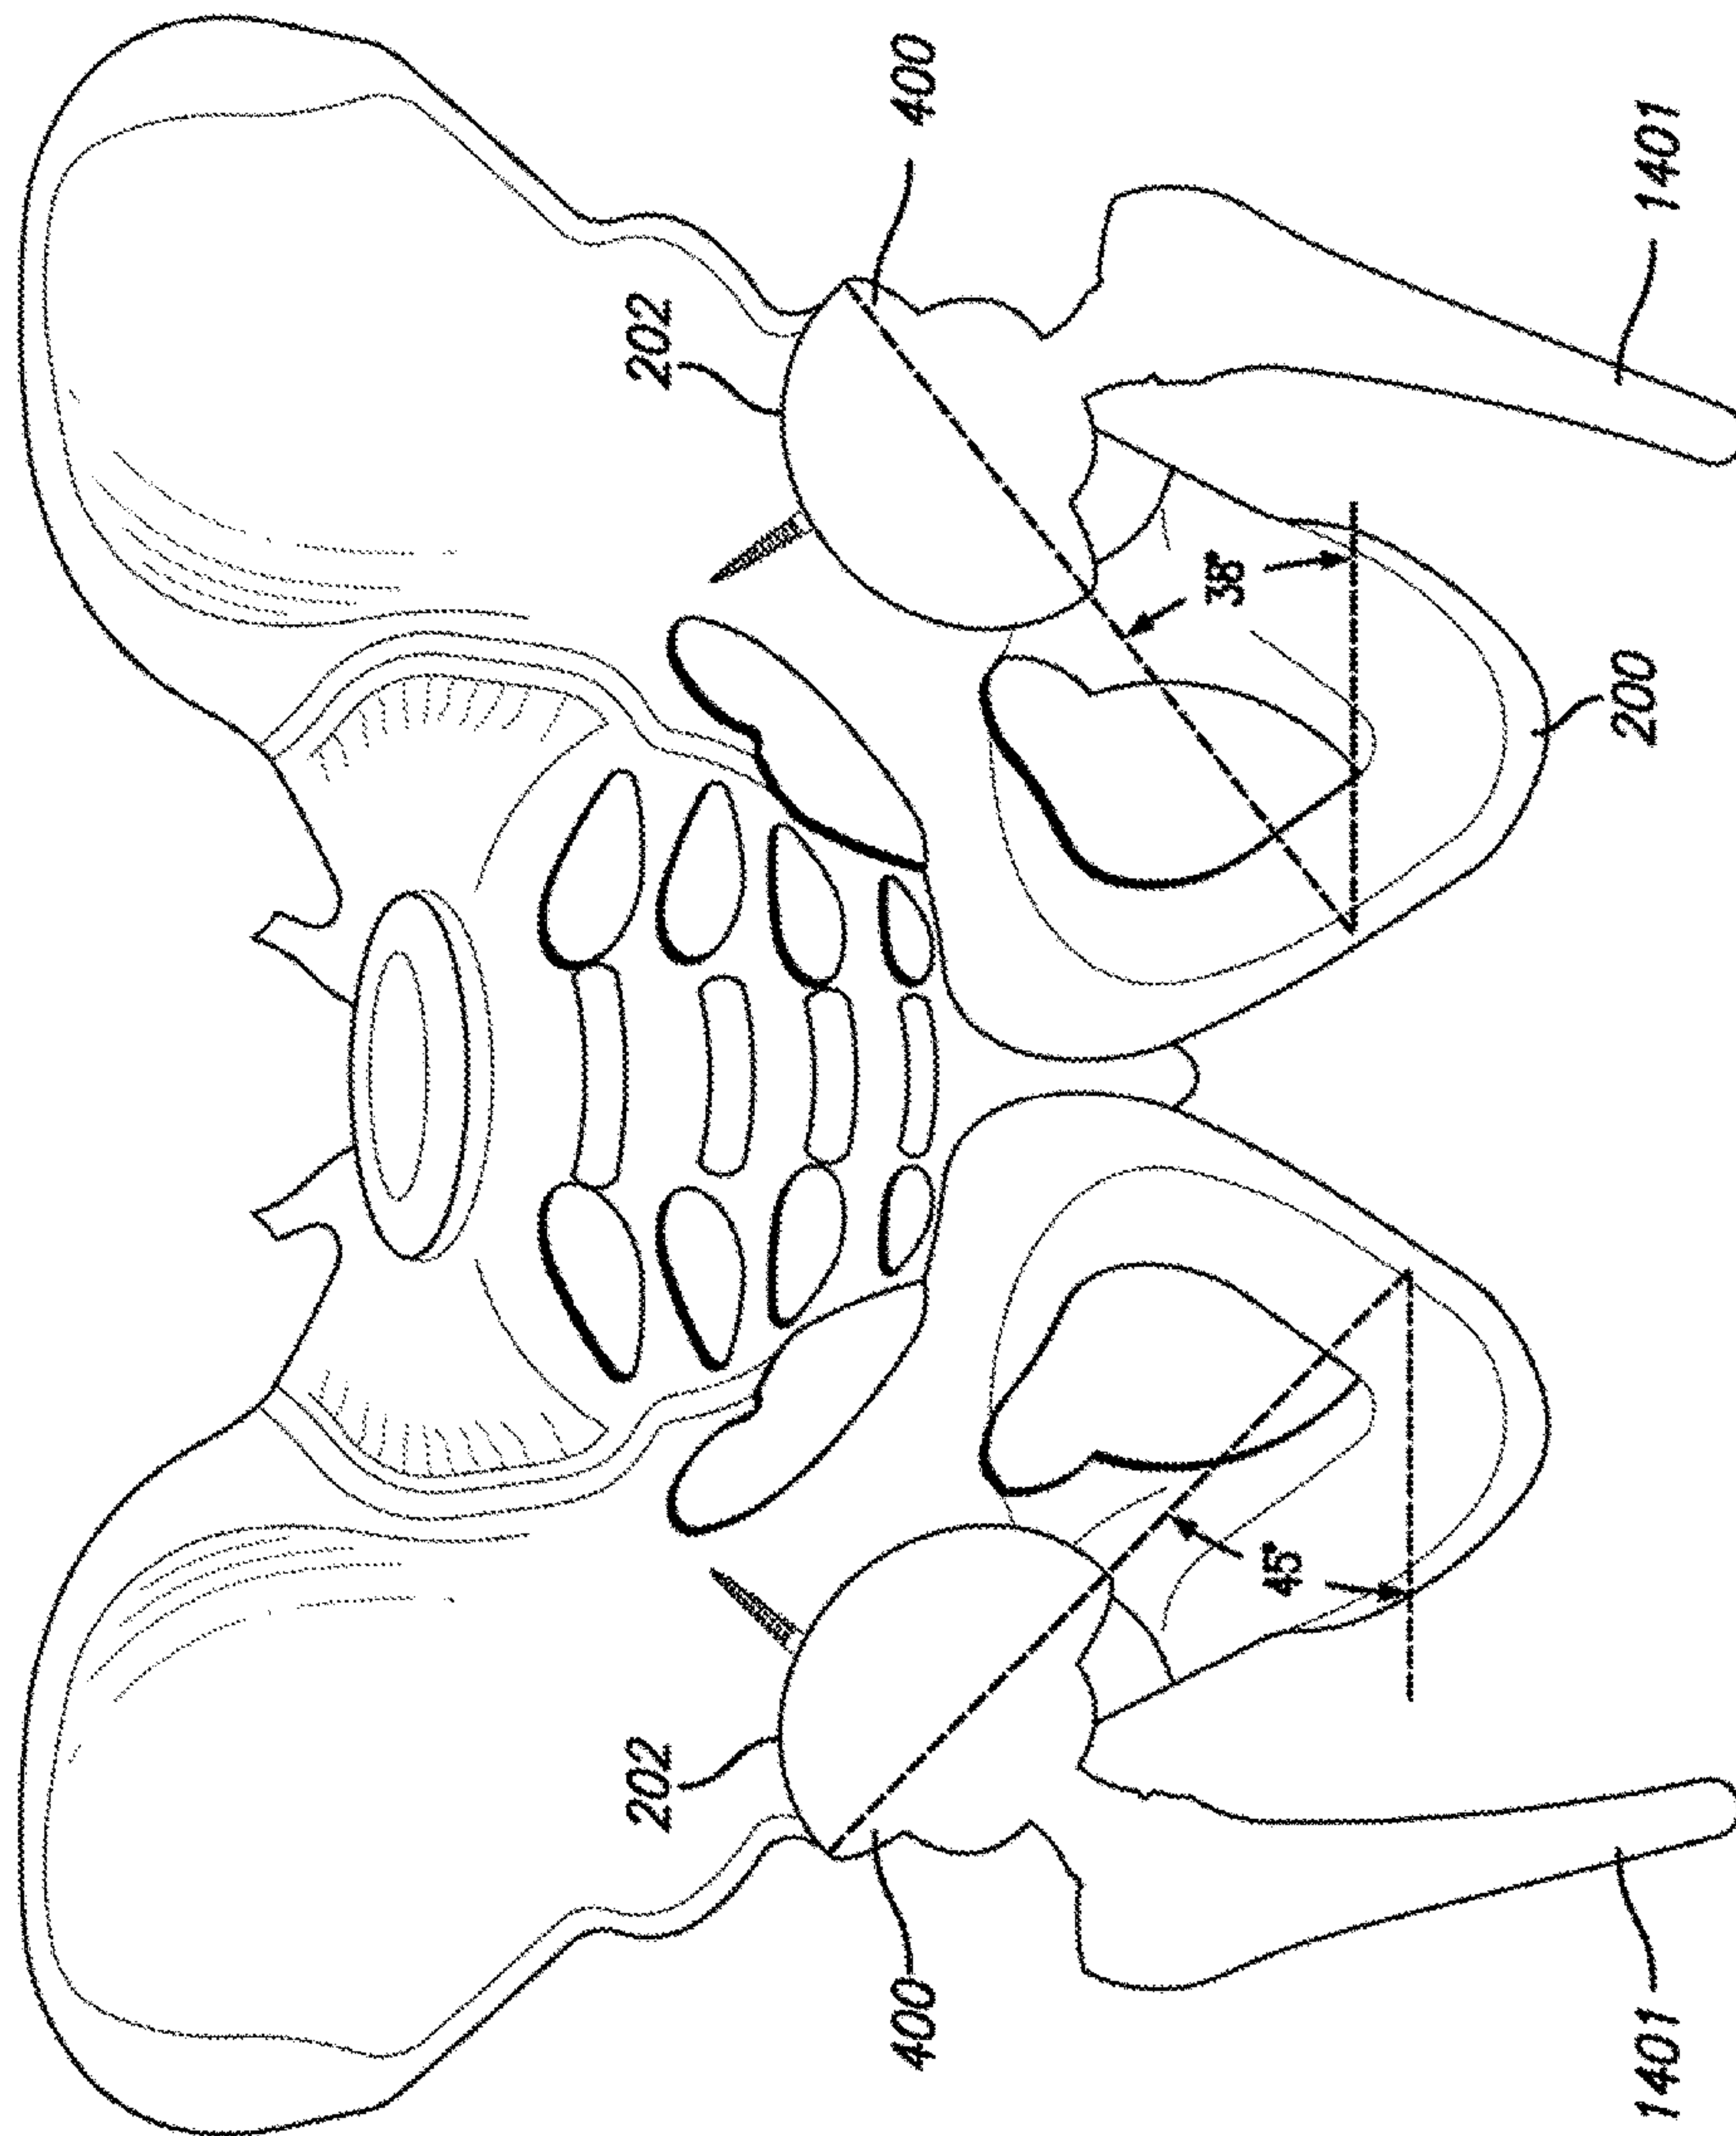


FIG. 1



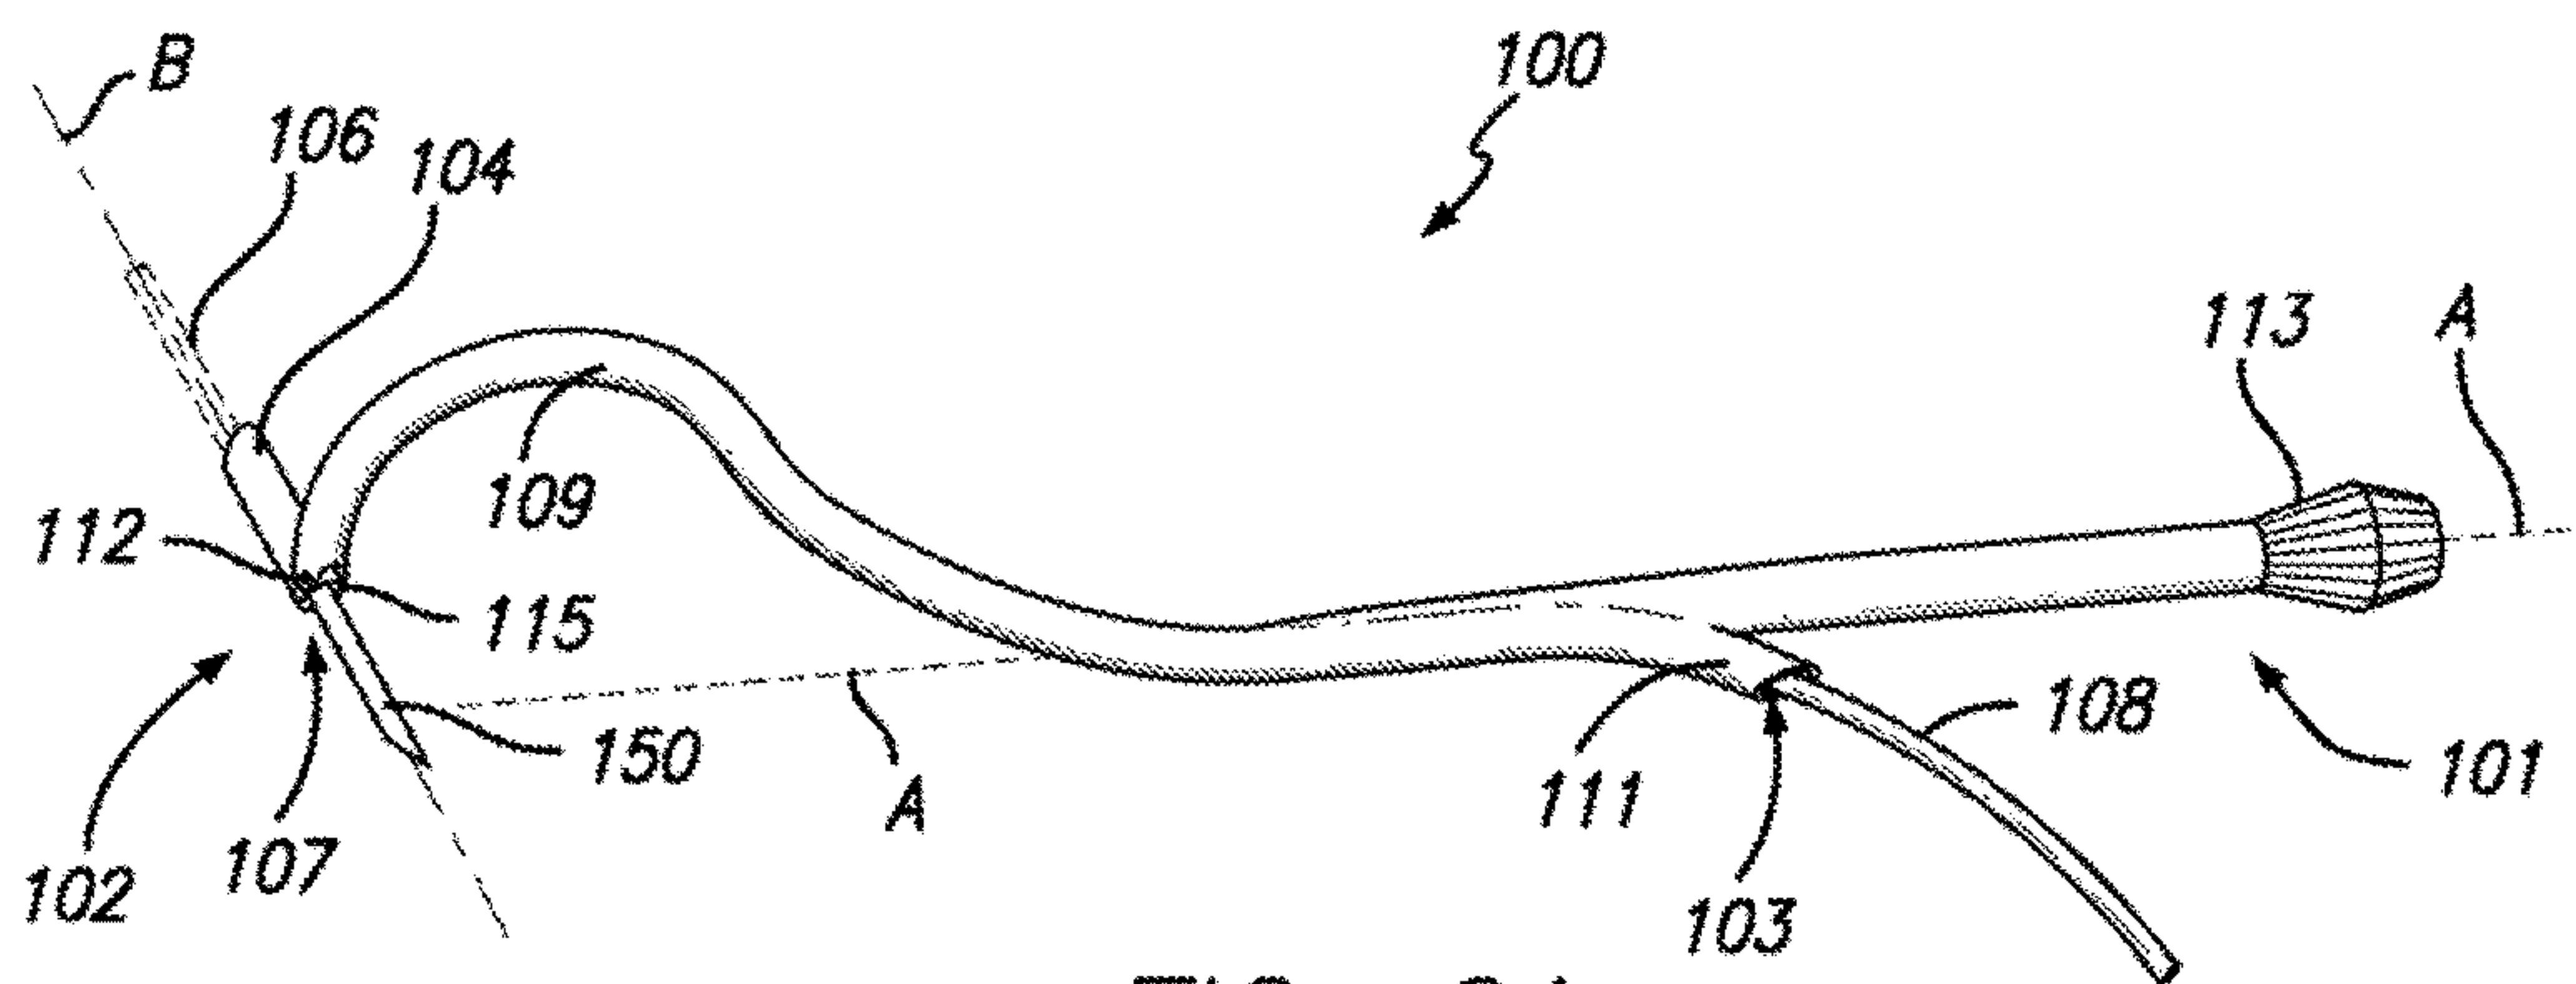


FIG. 2A

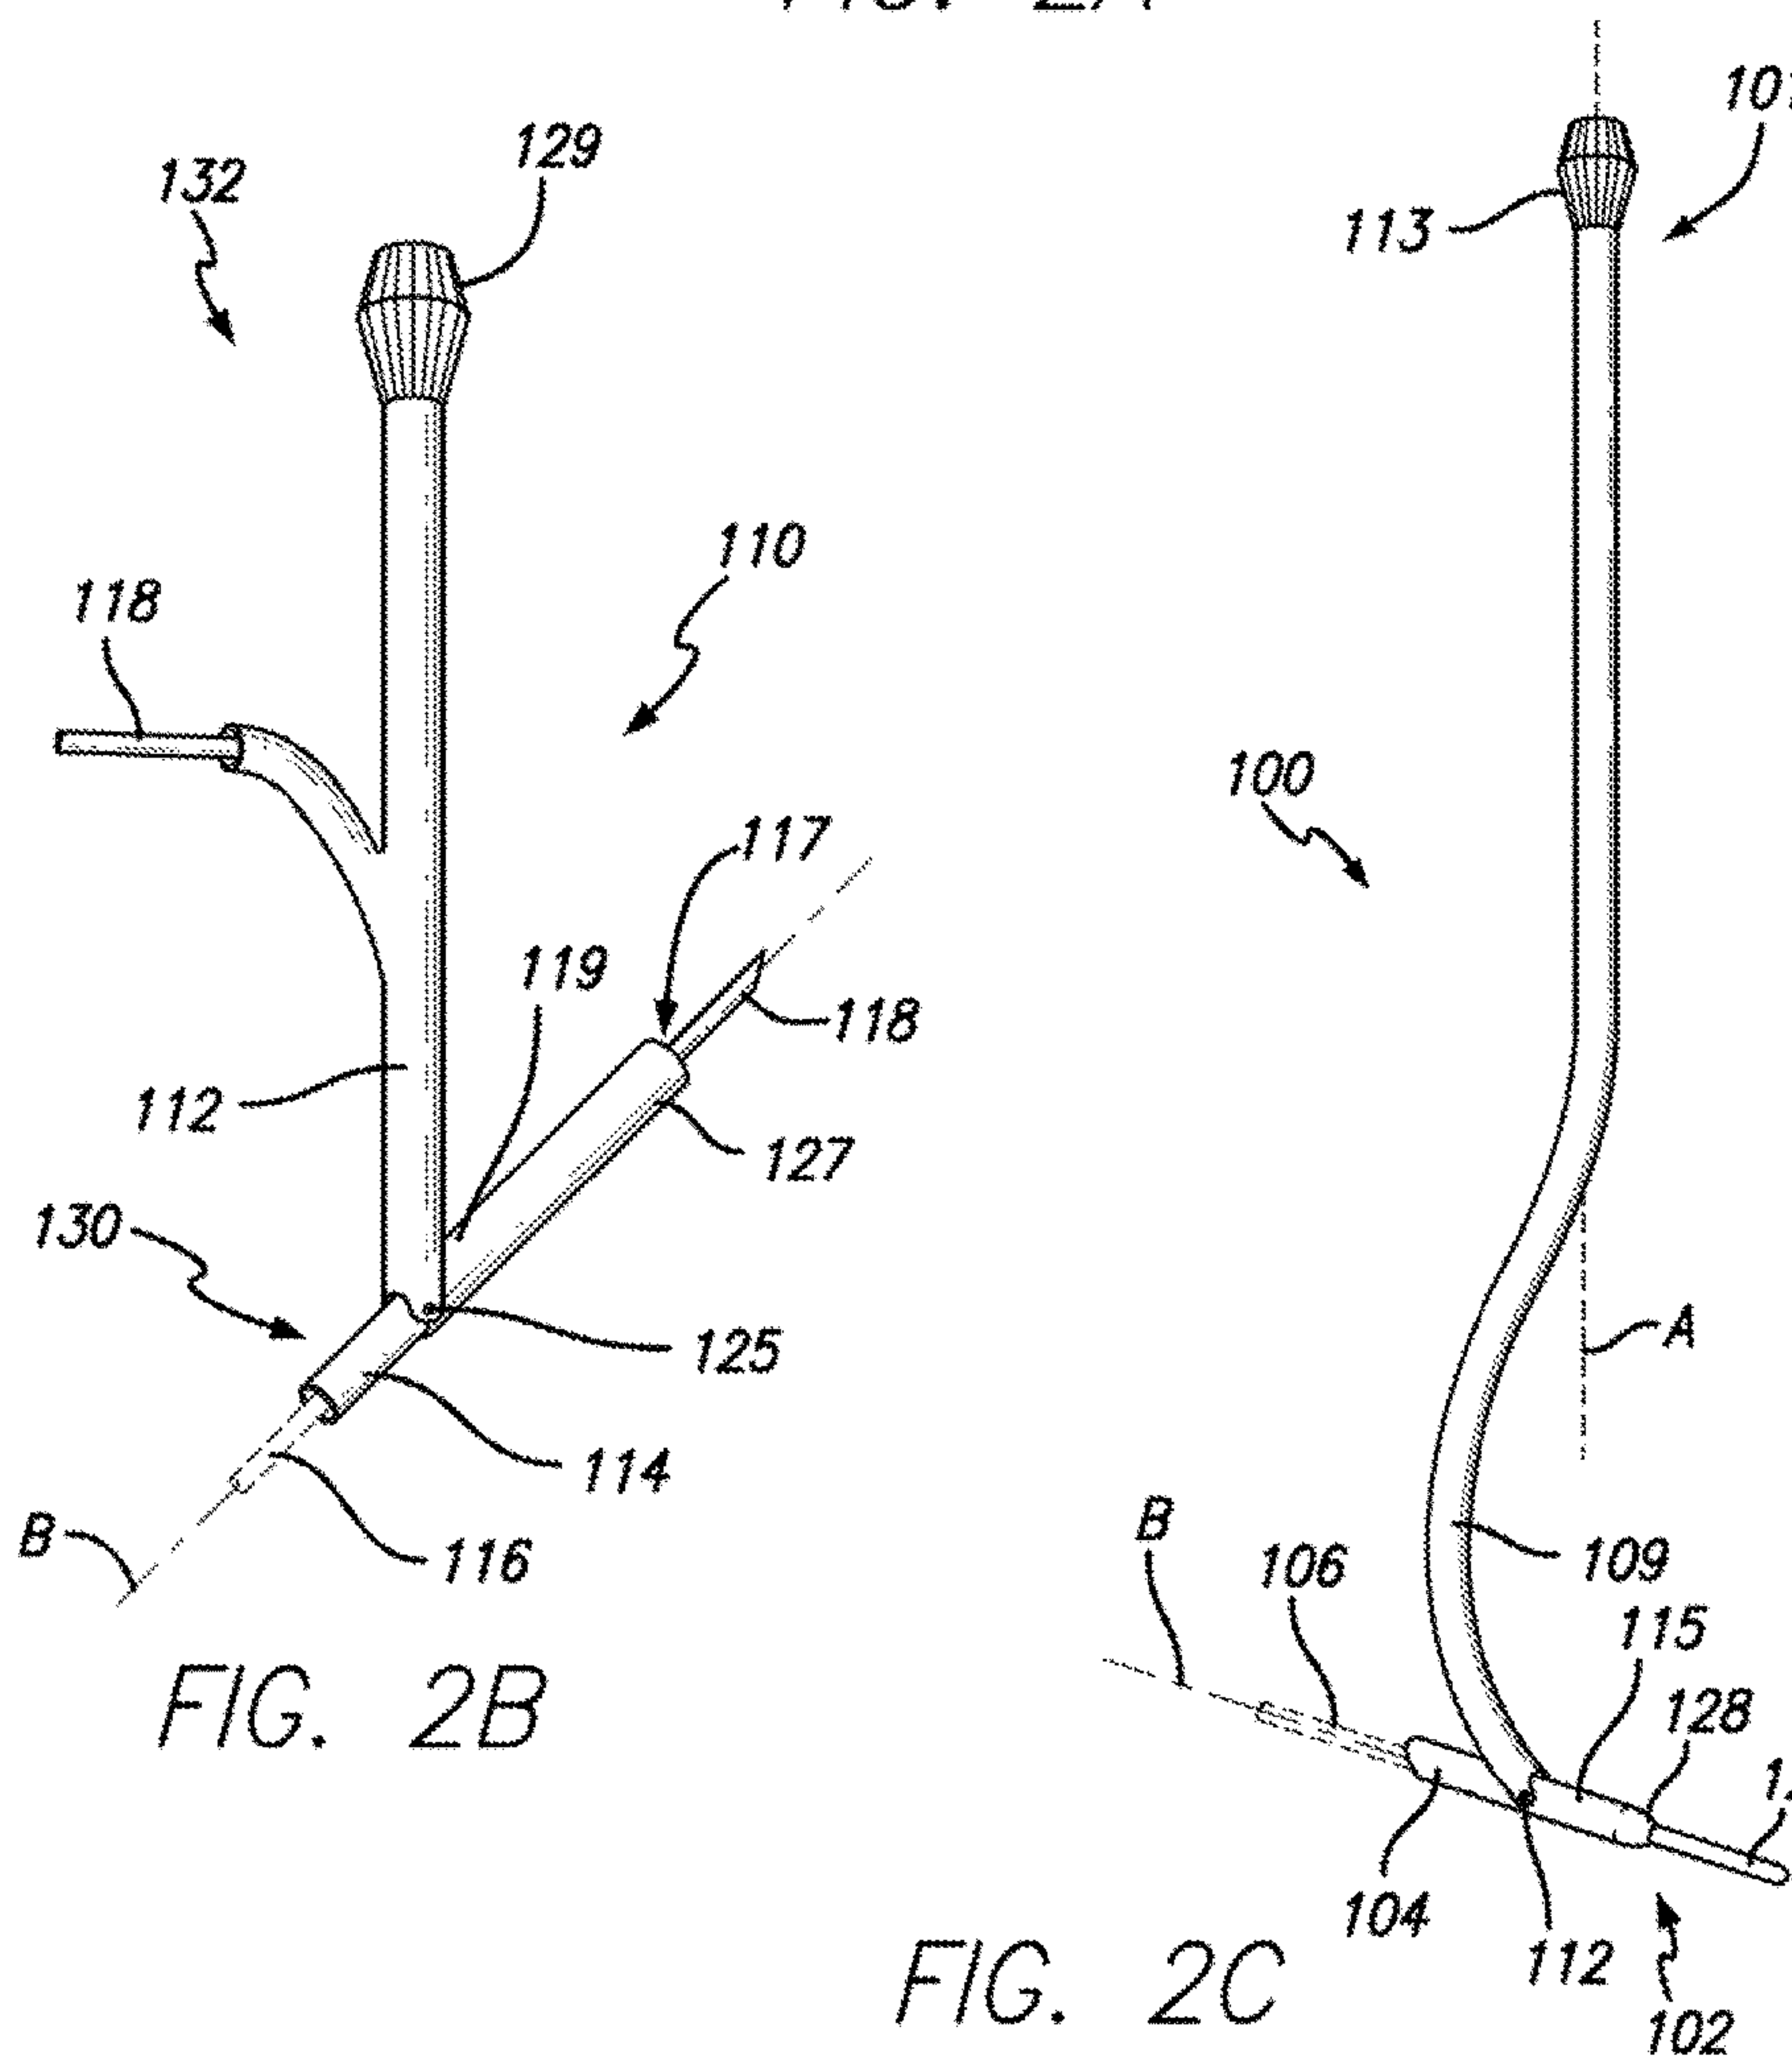
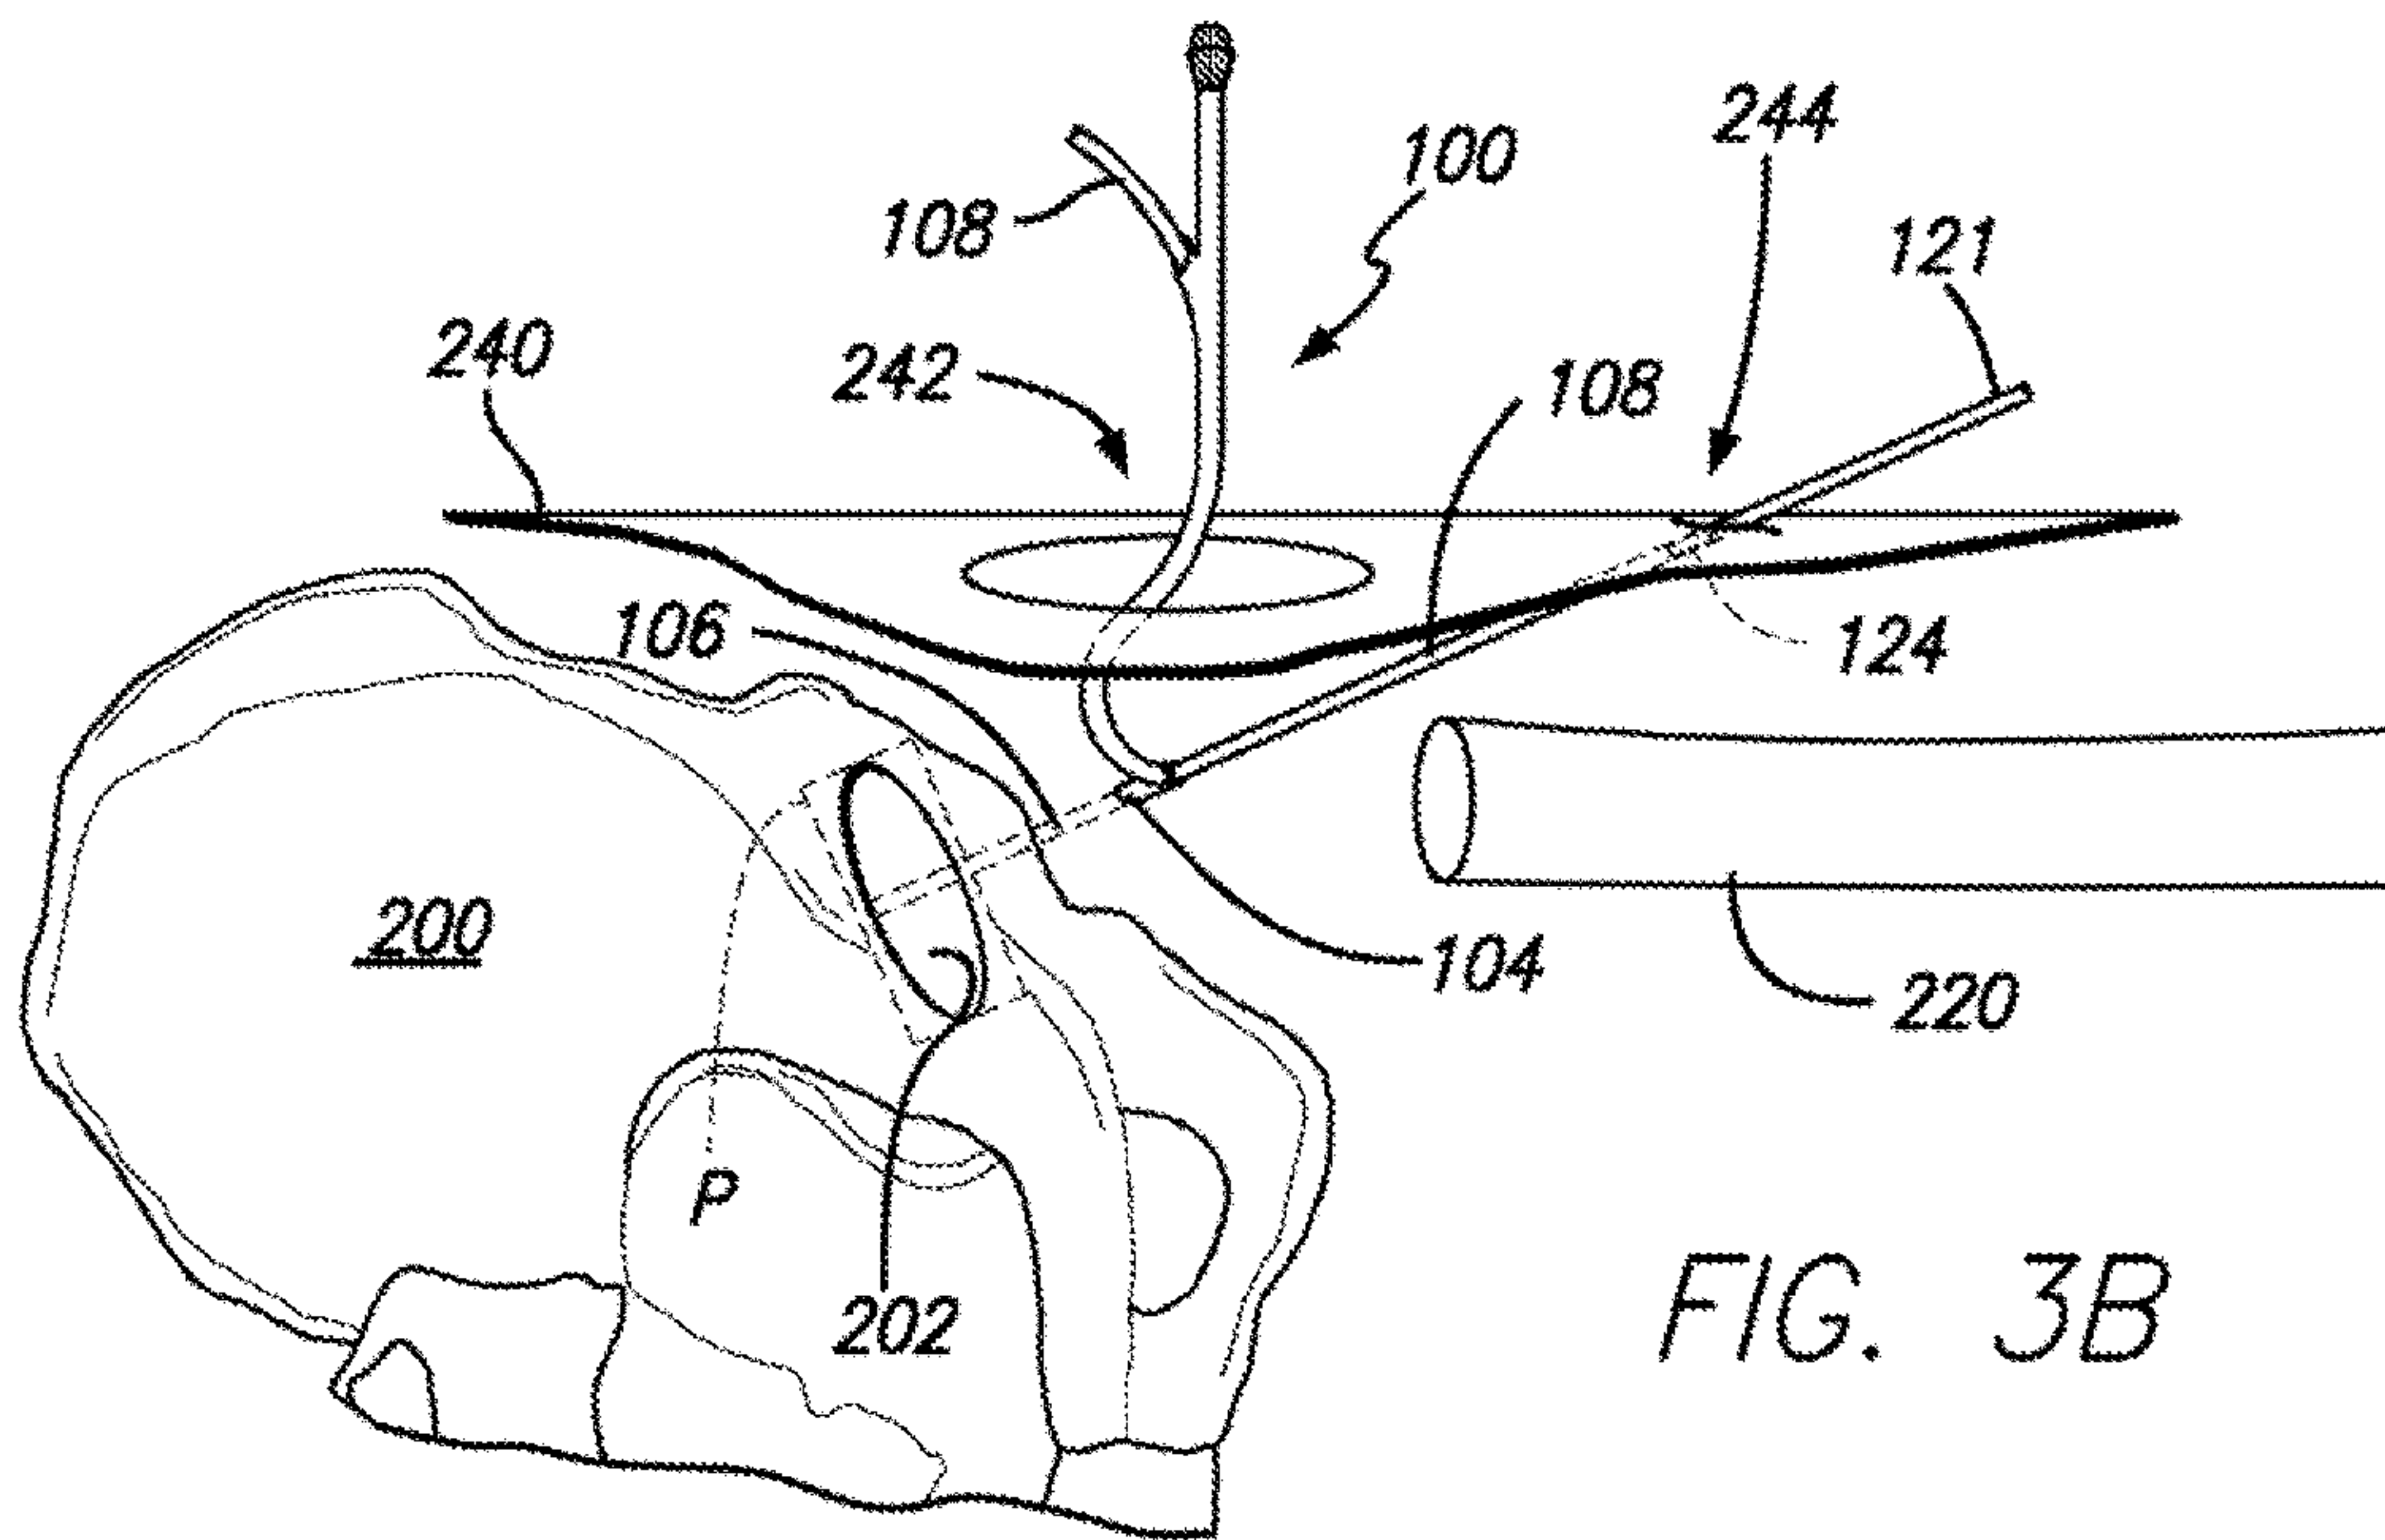
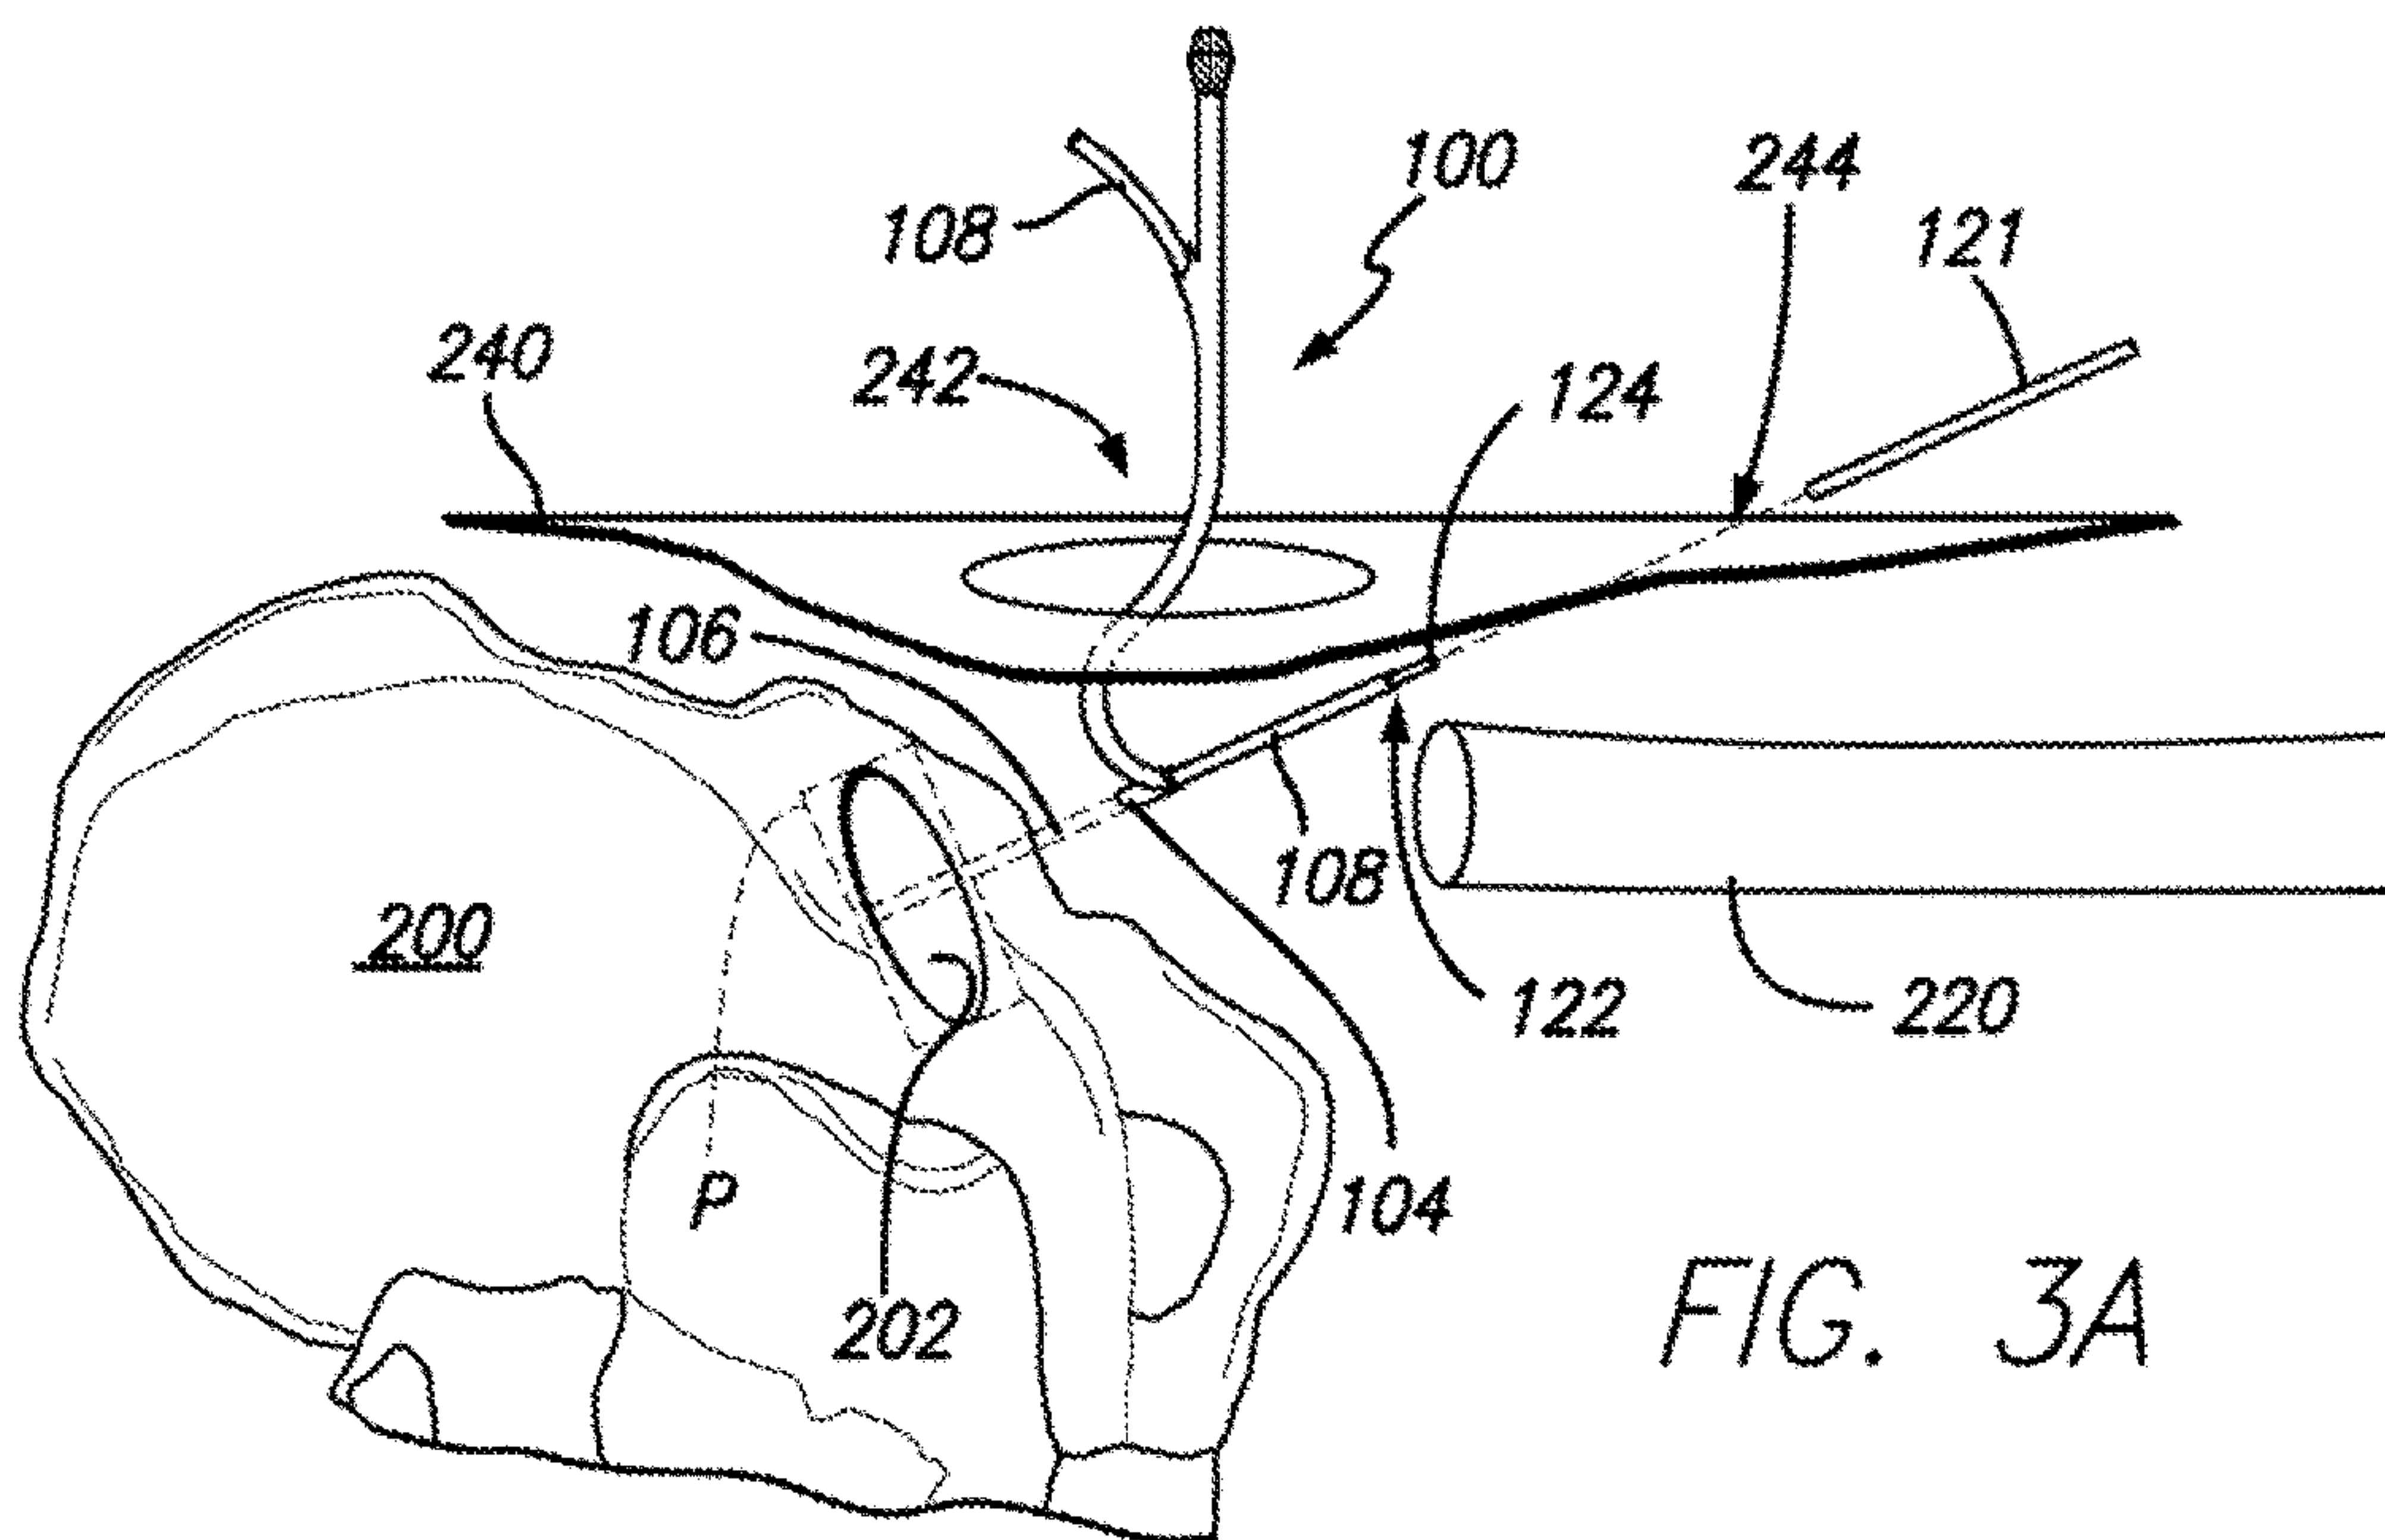


FIG. 2B

FIG. 2C



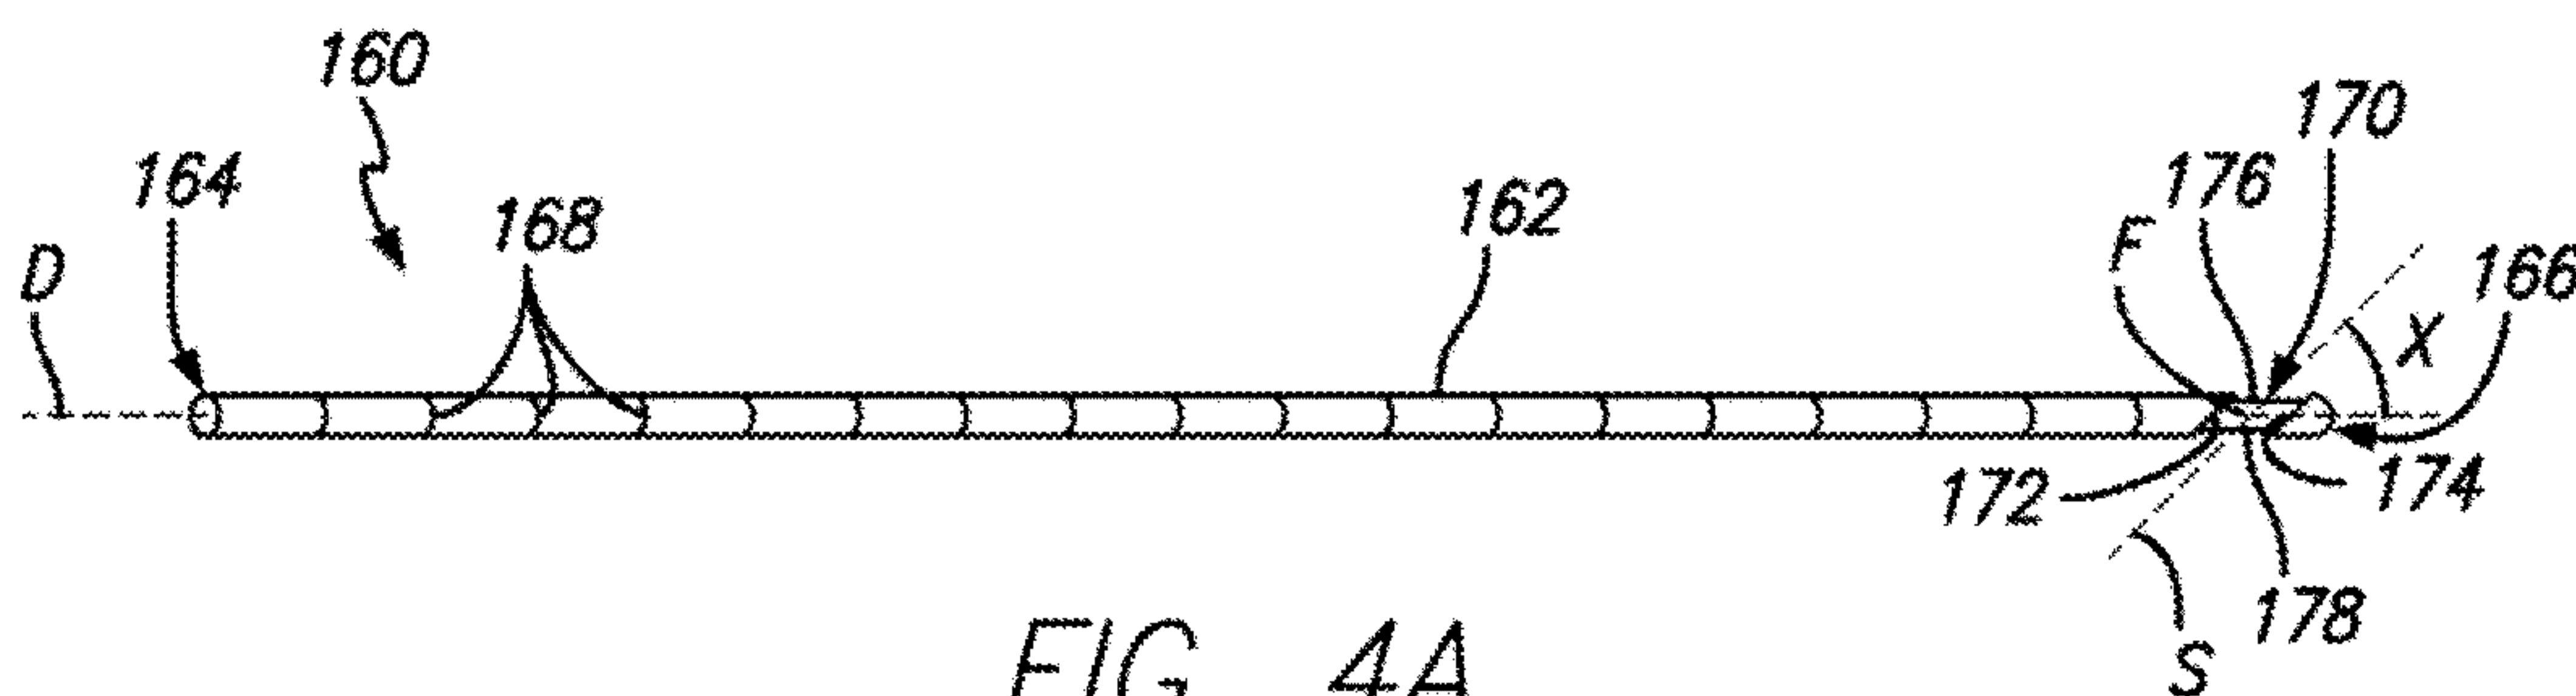


FIG. 4A

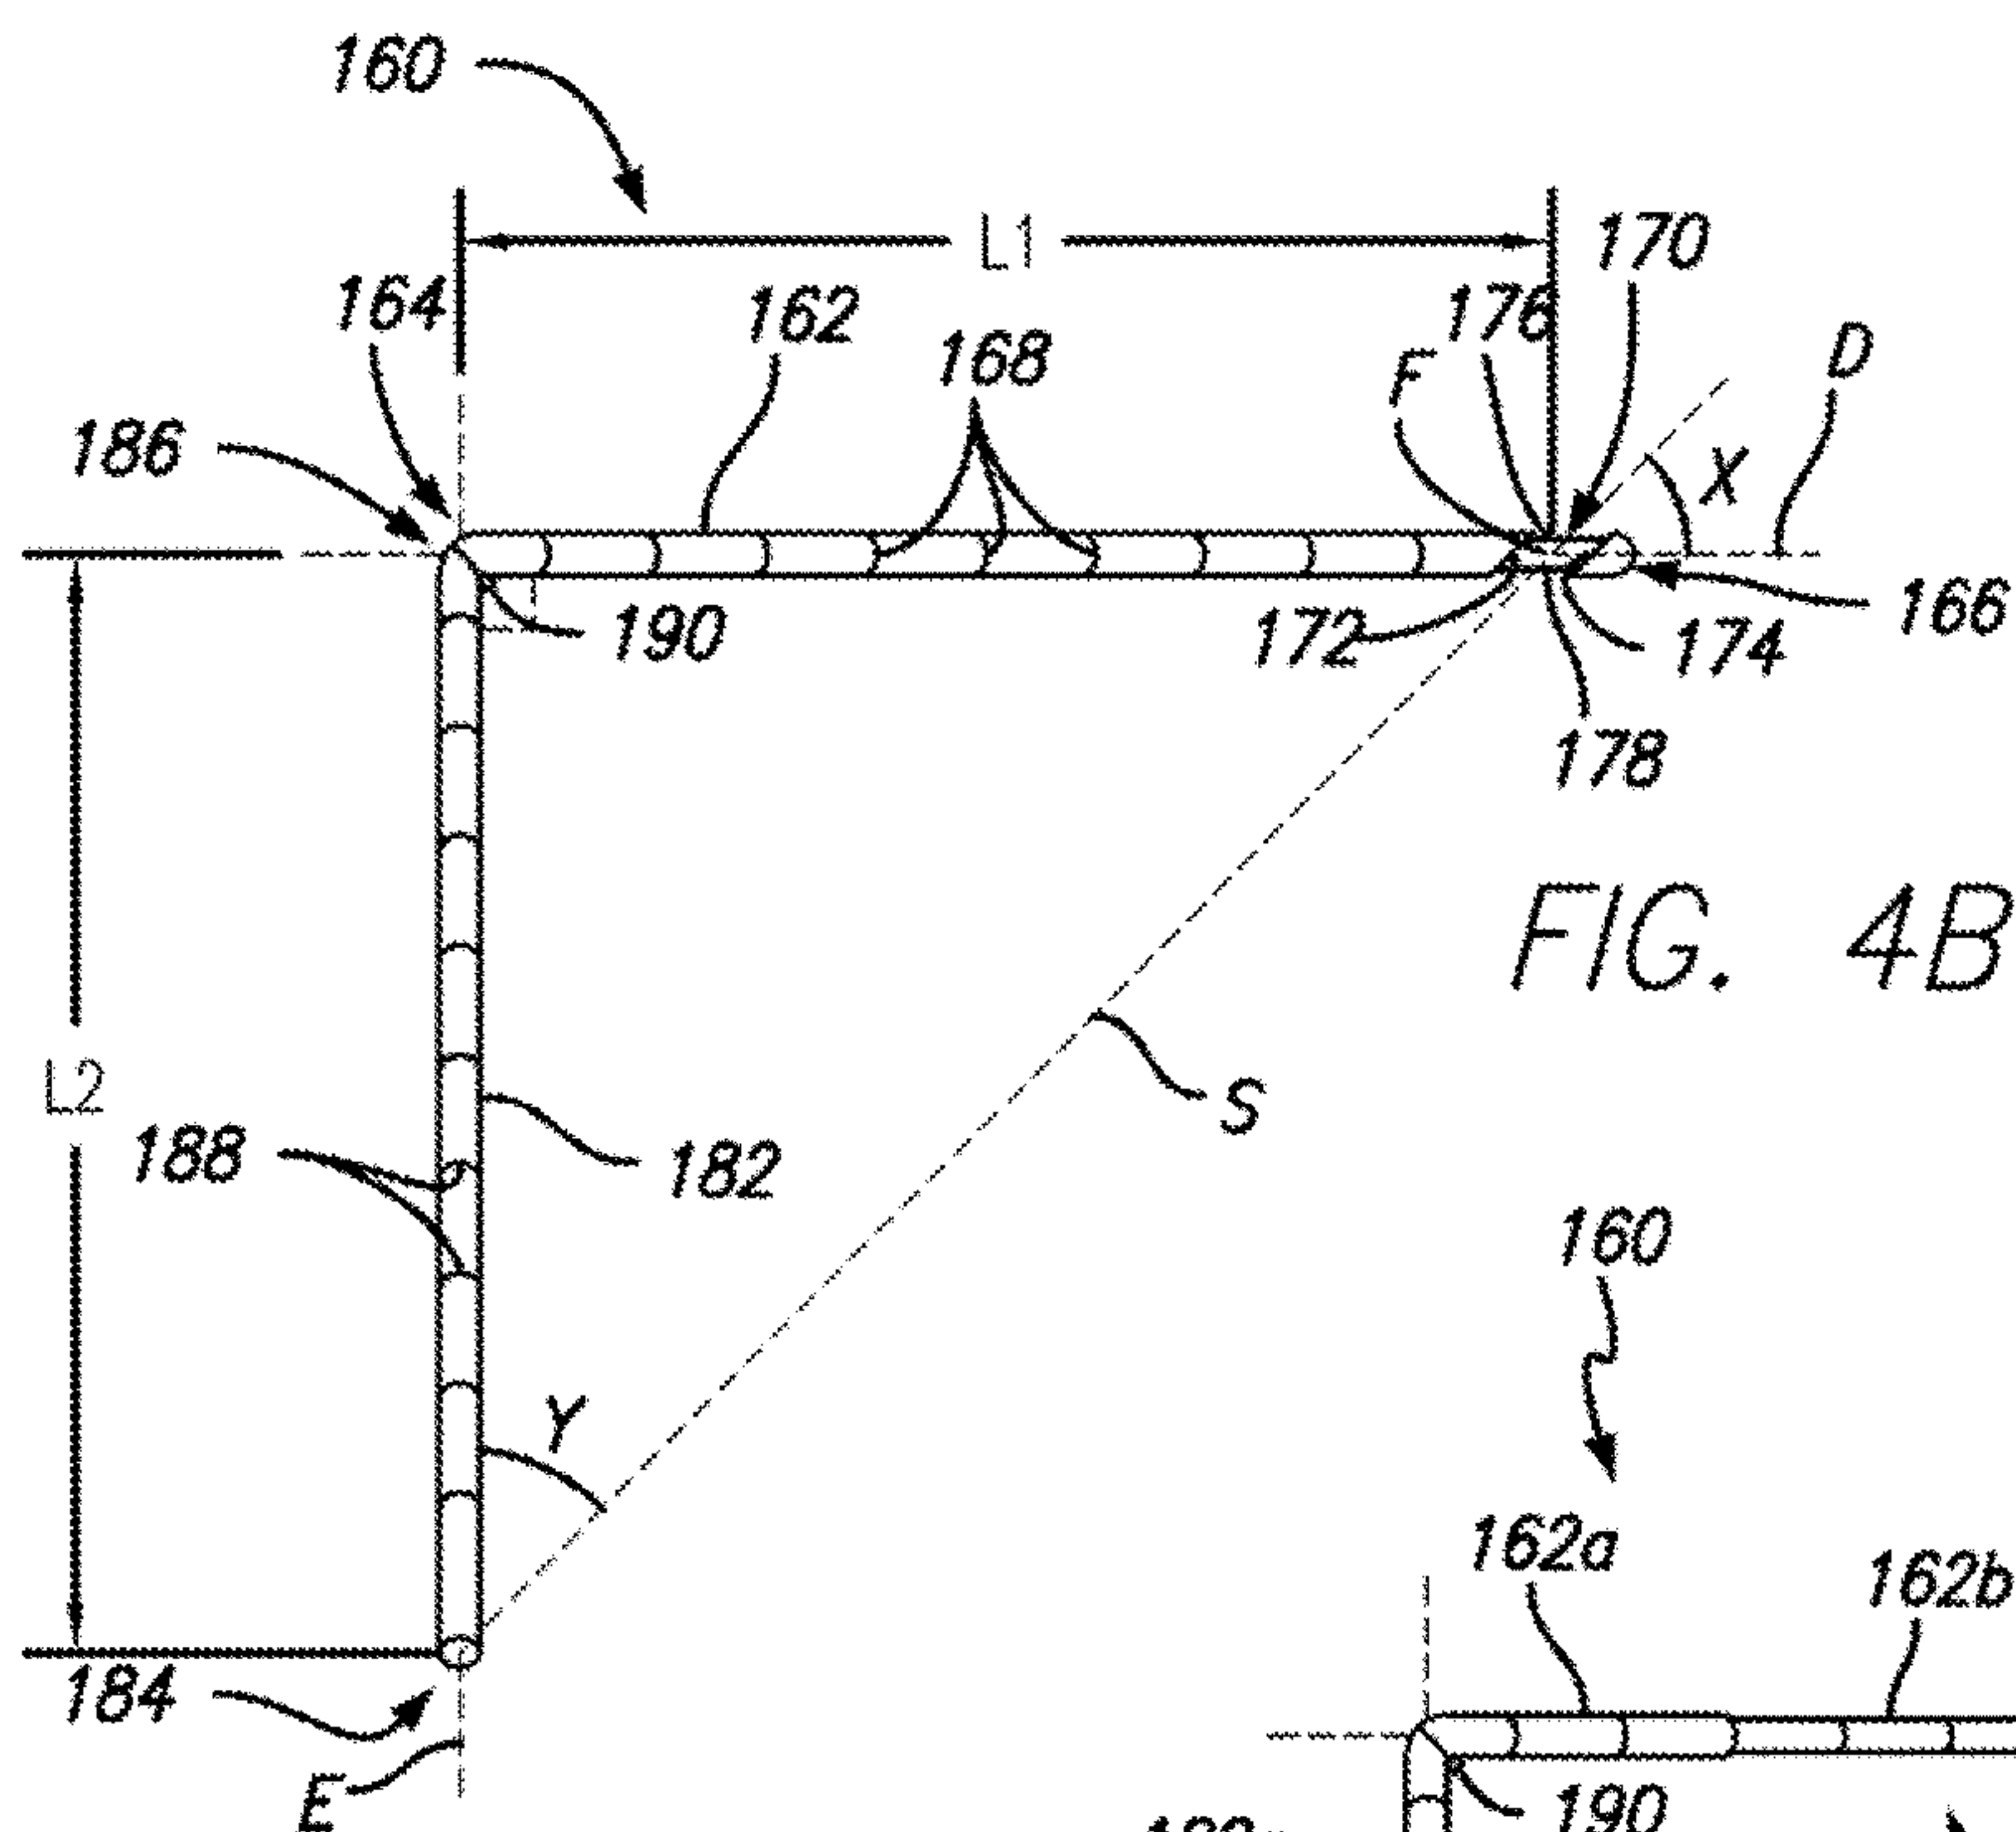


FIG. 4B

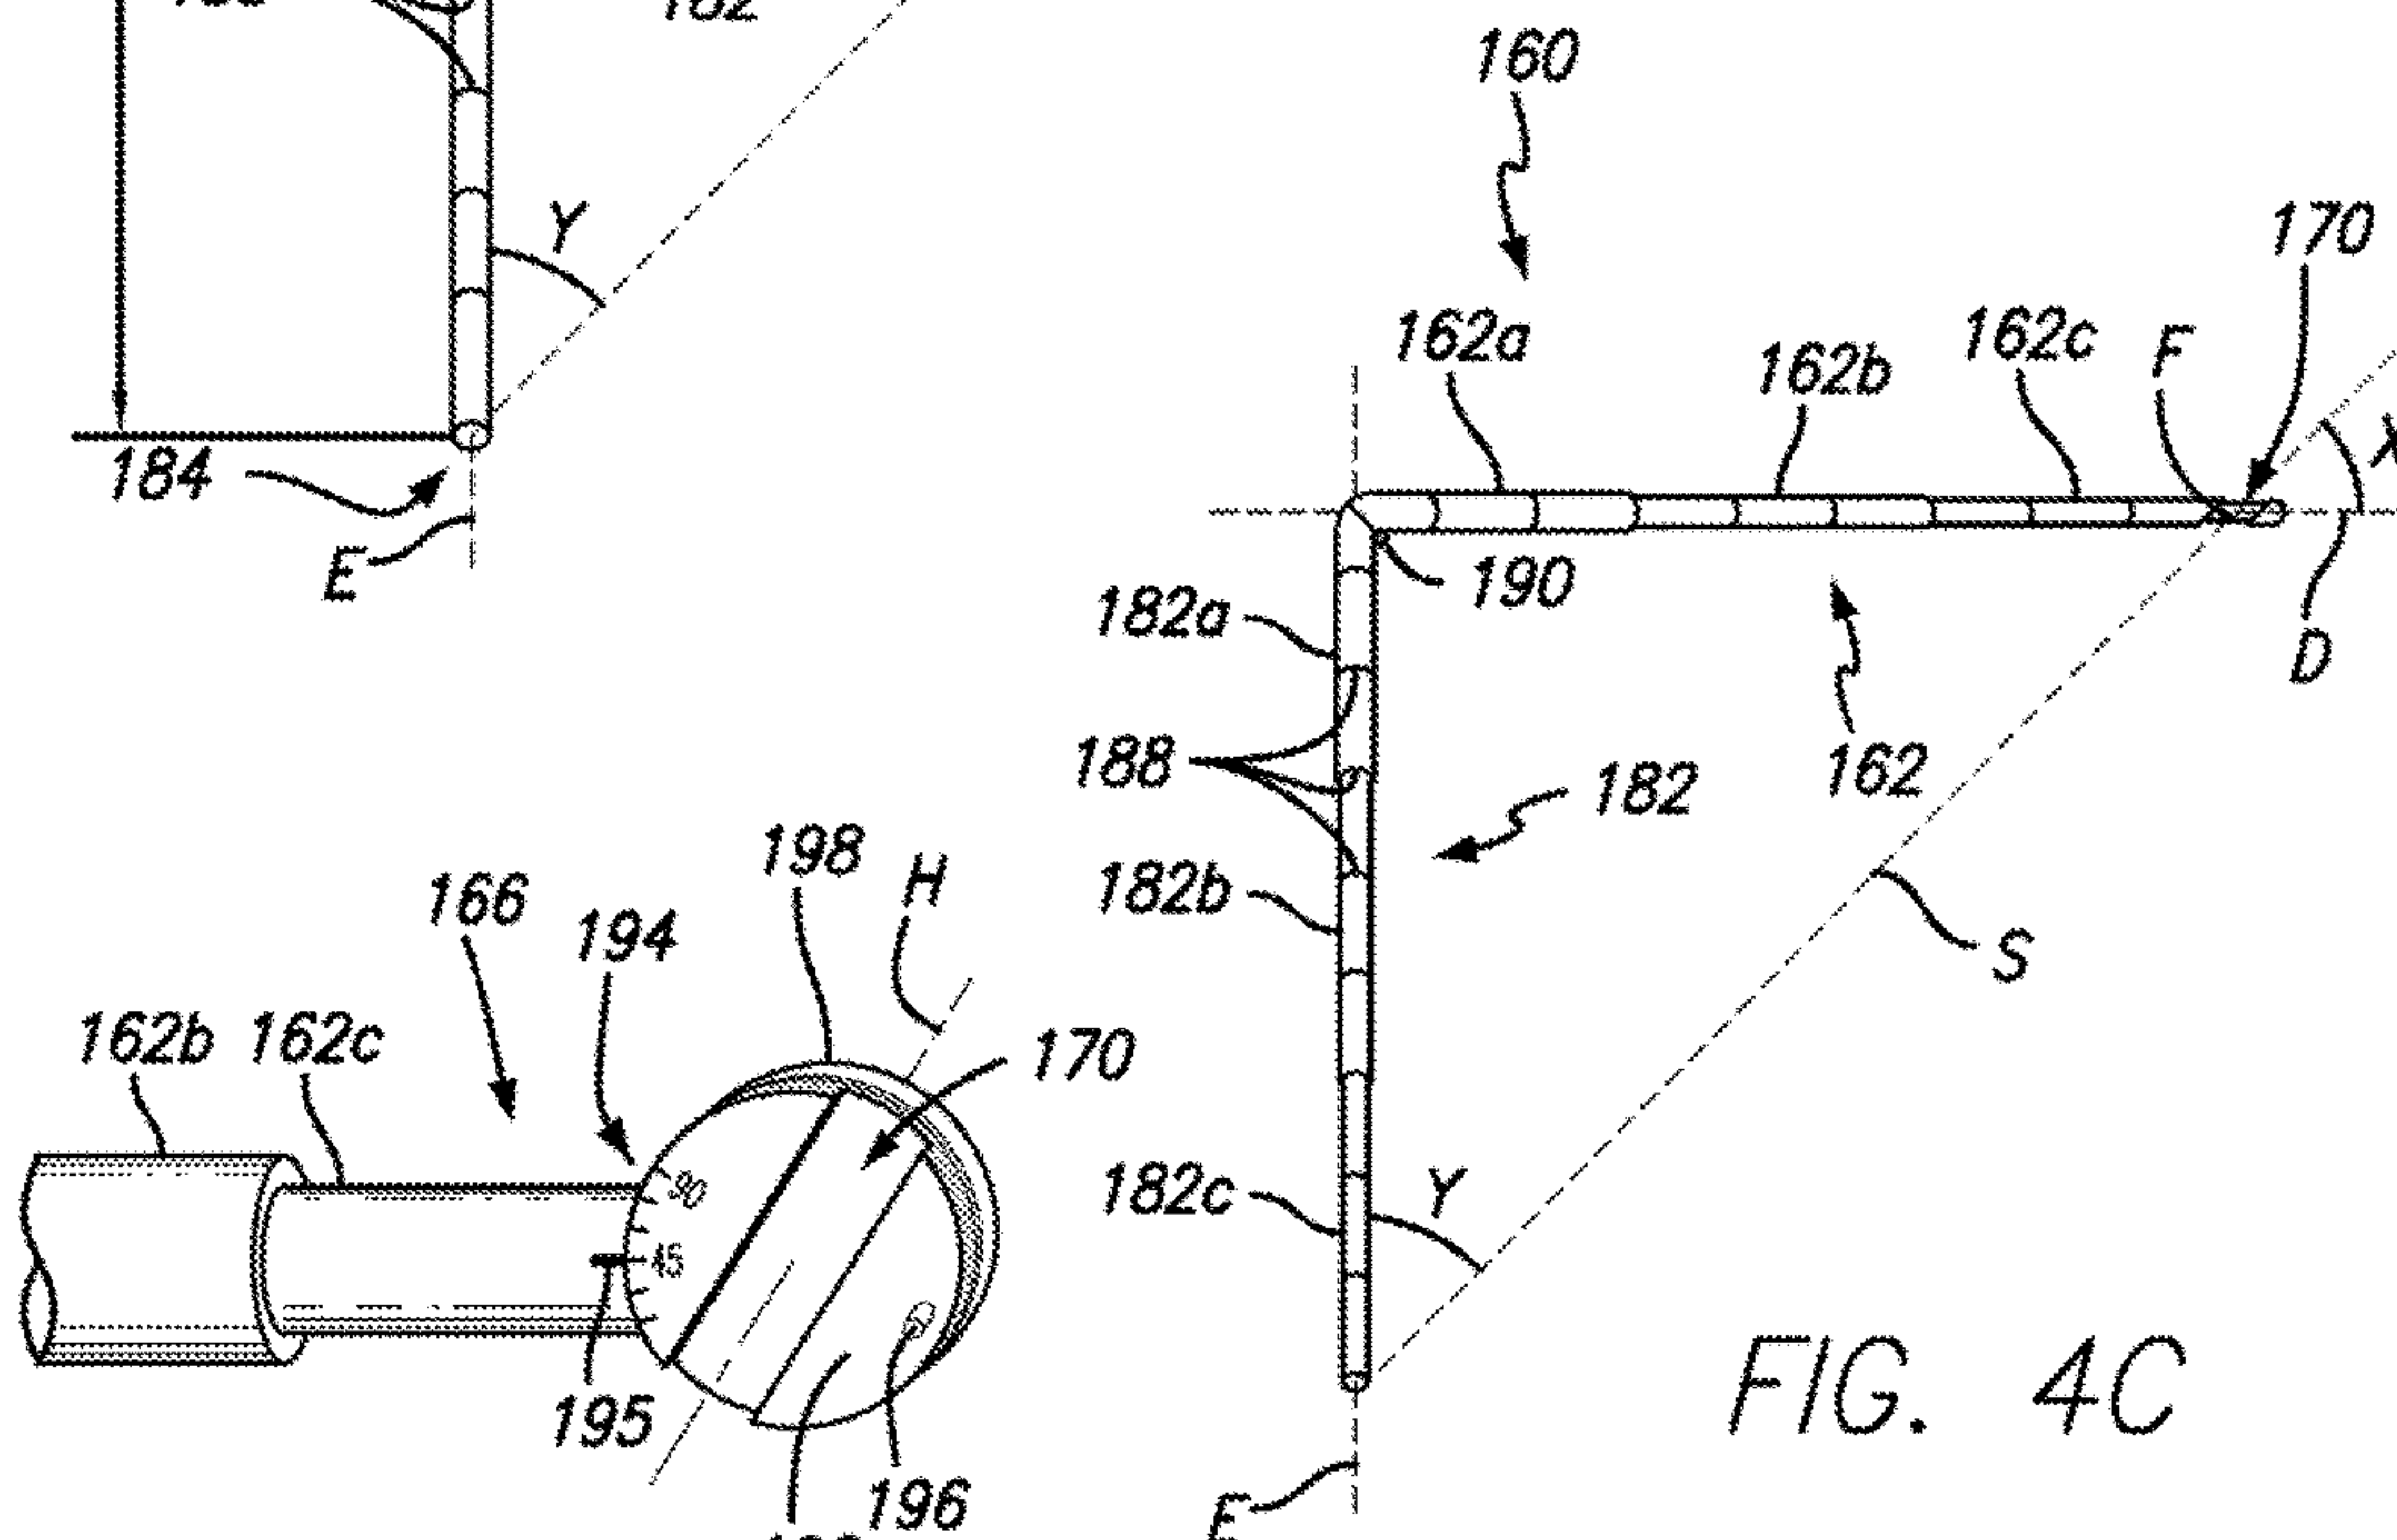


FIG. 4C

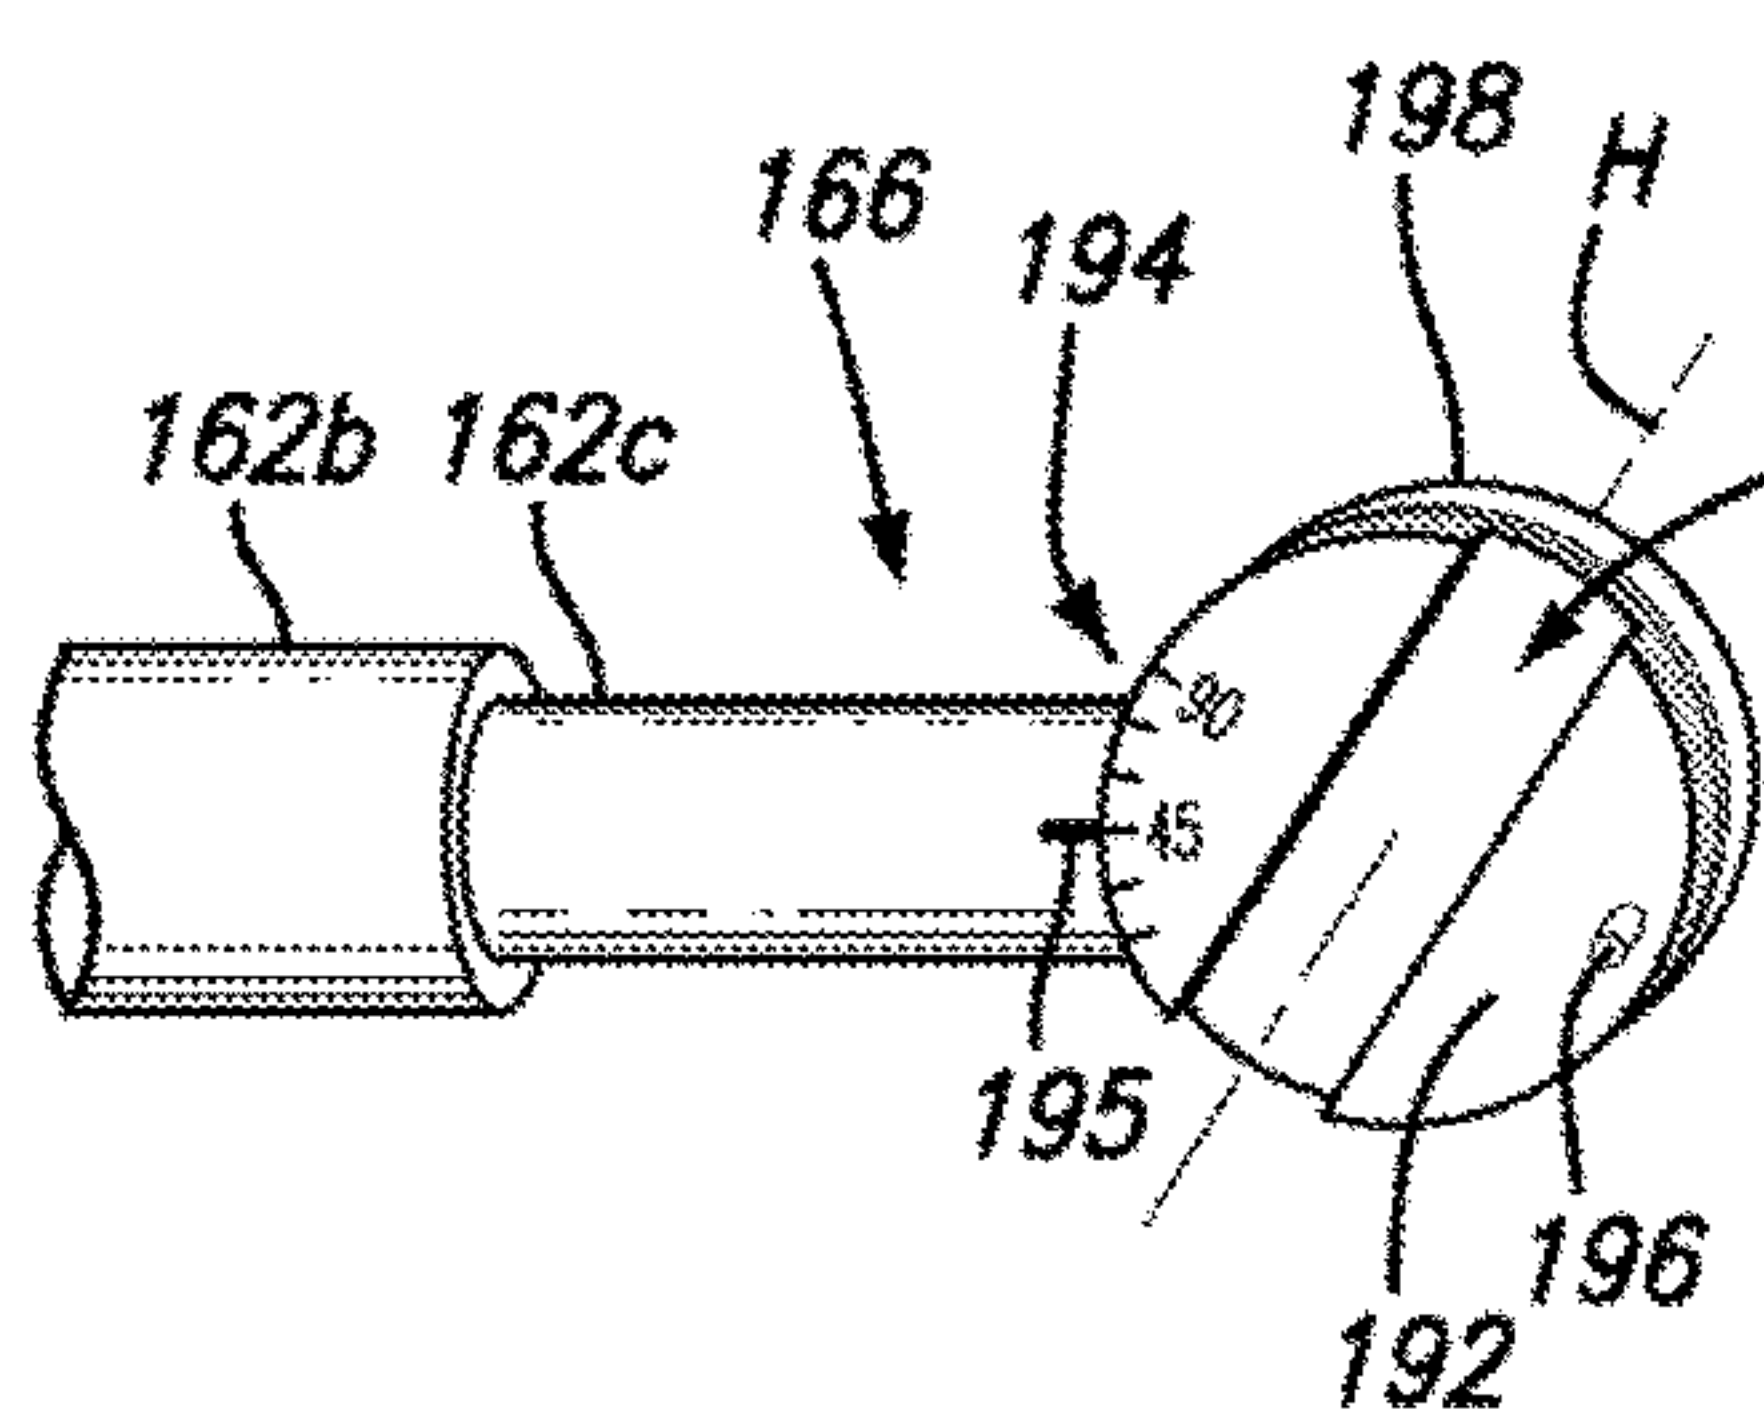
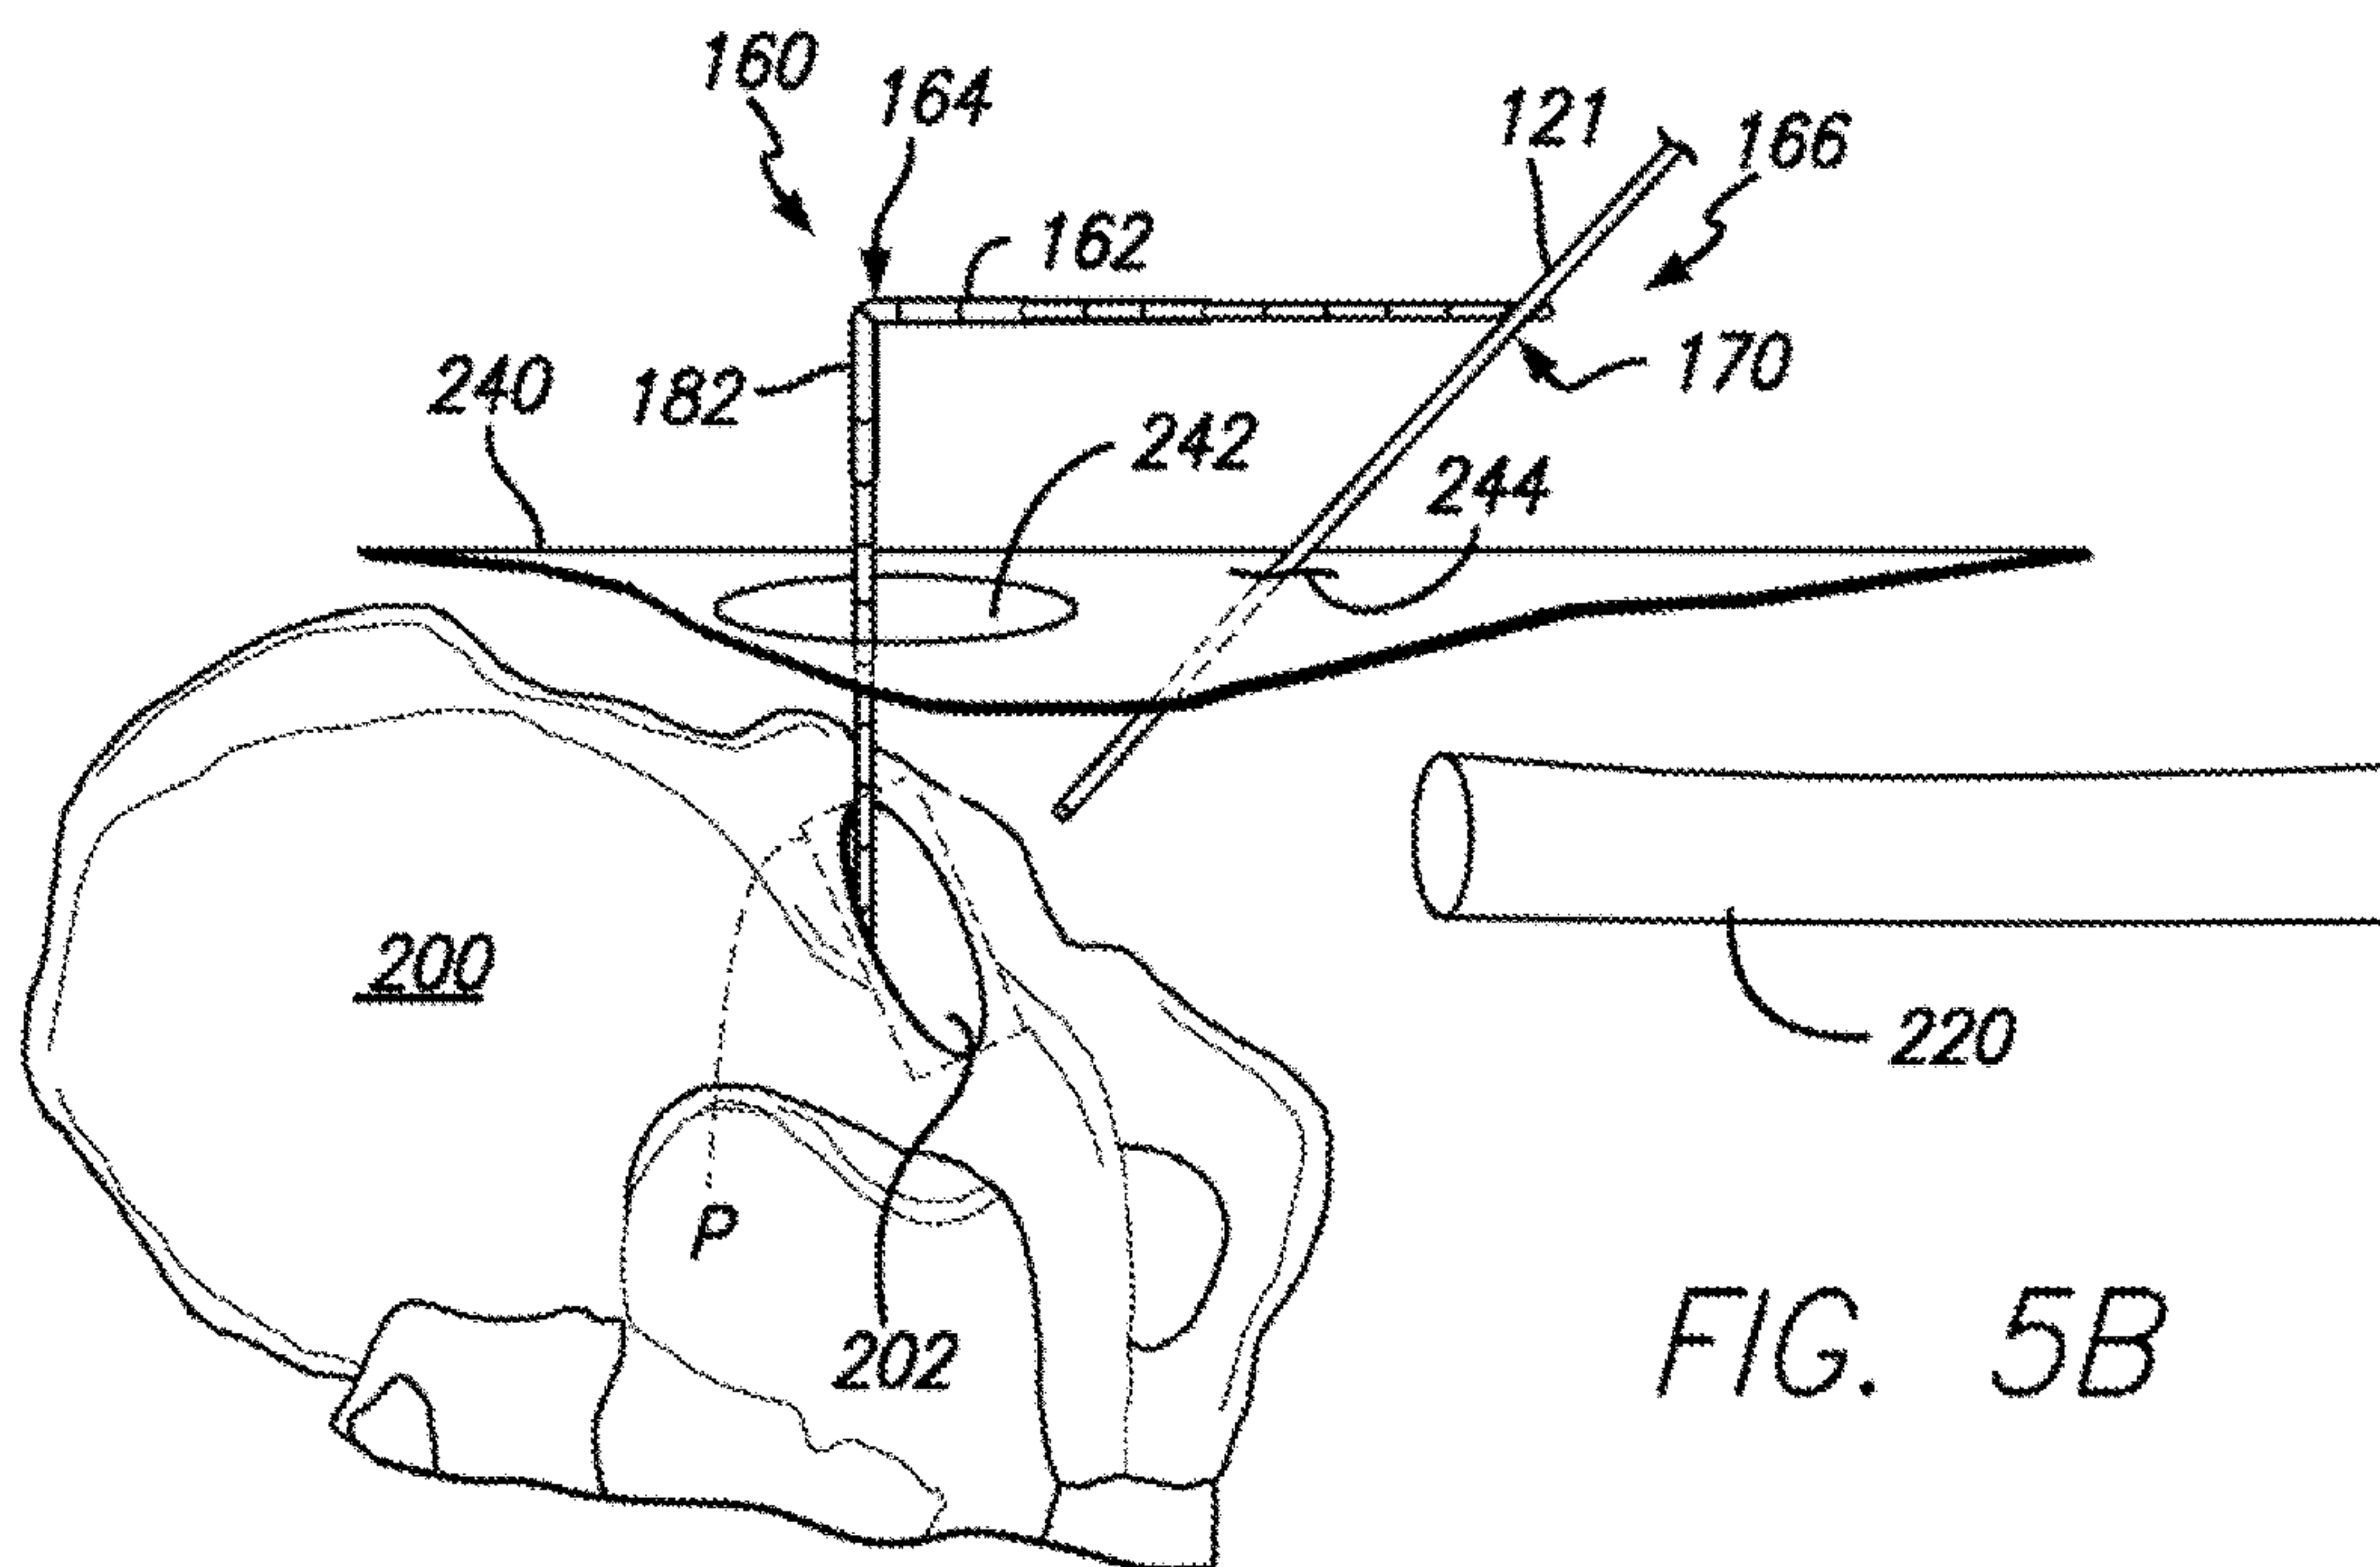
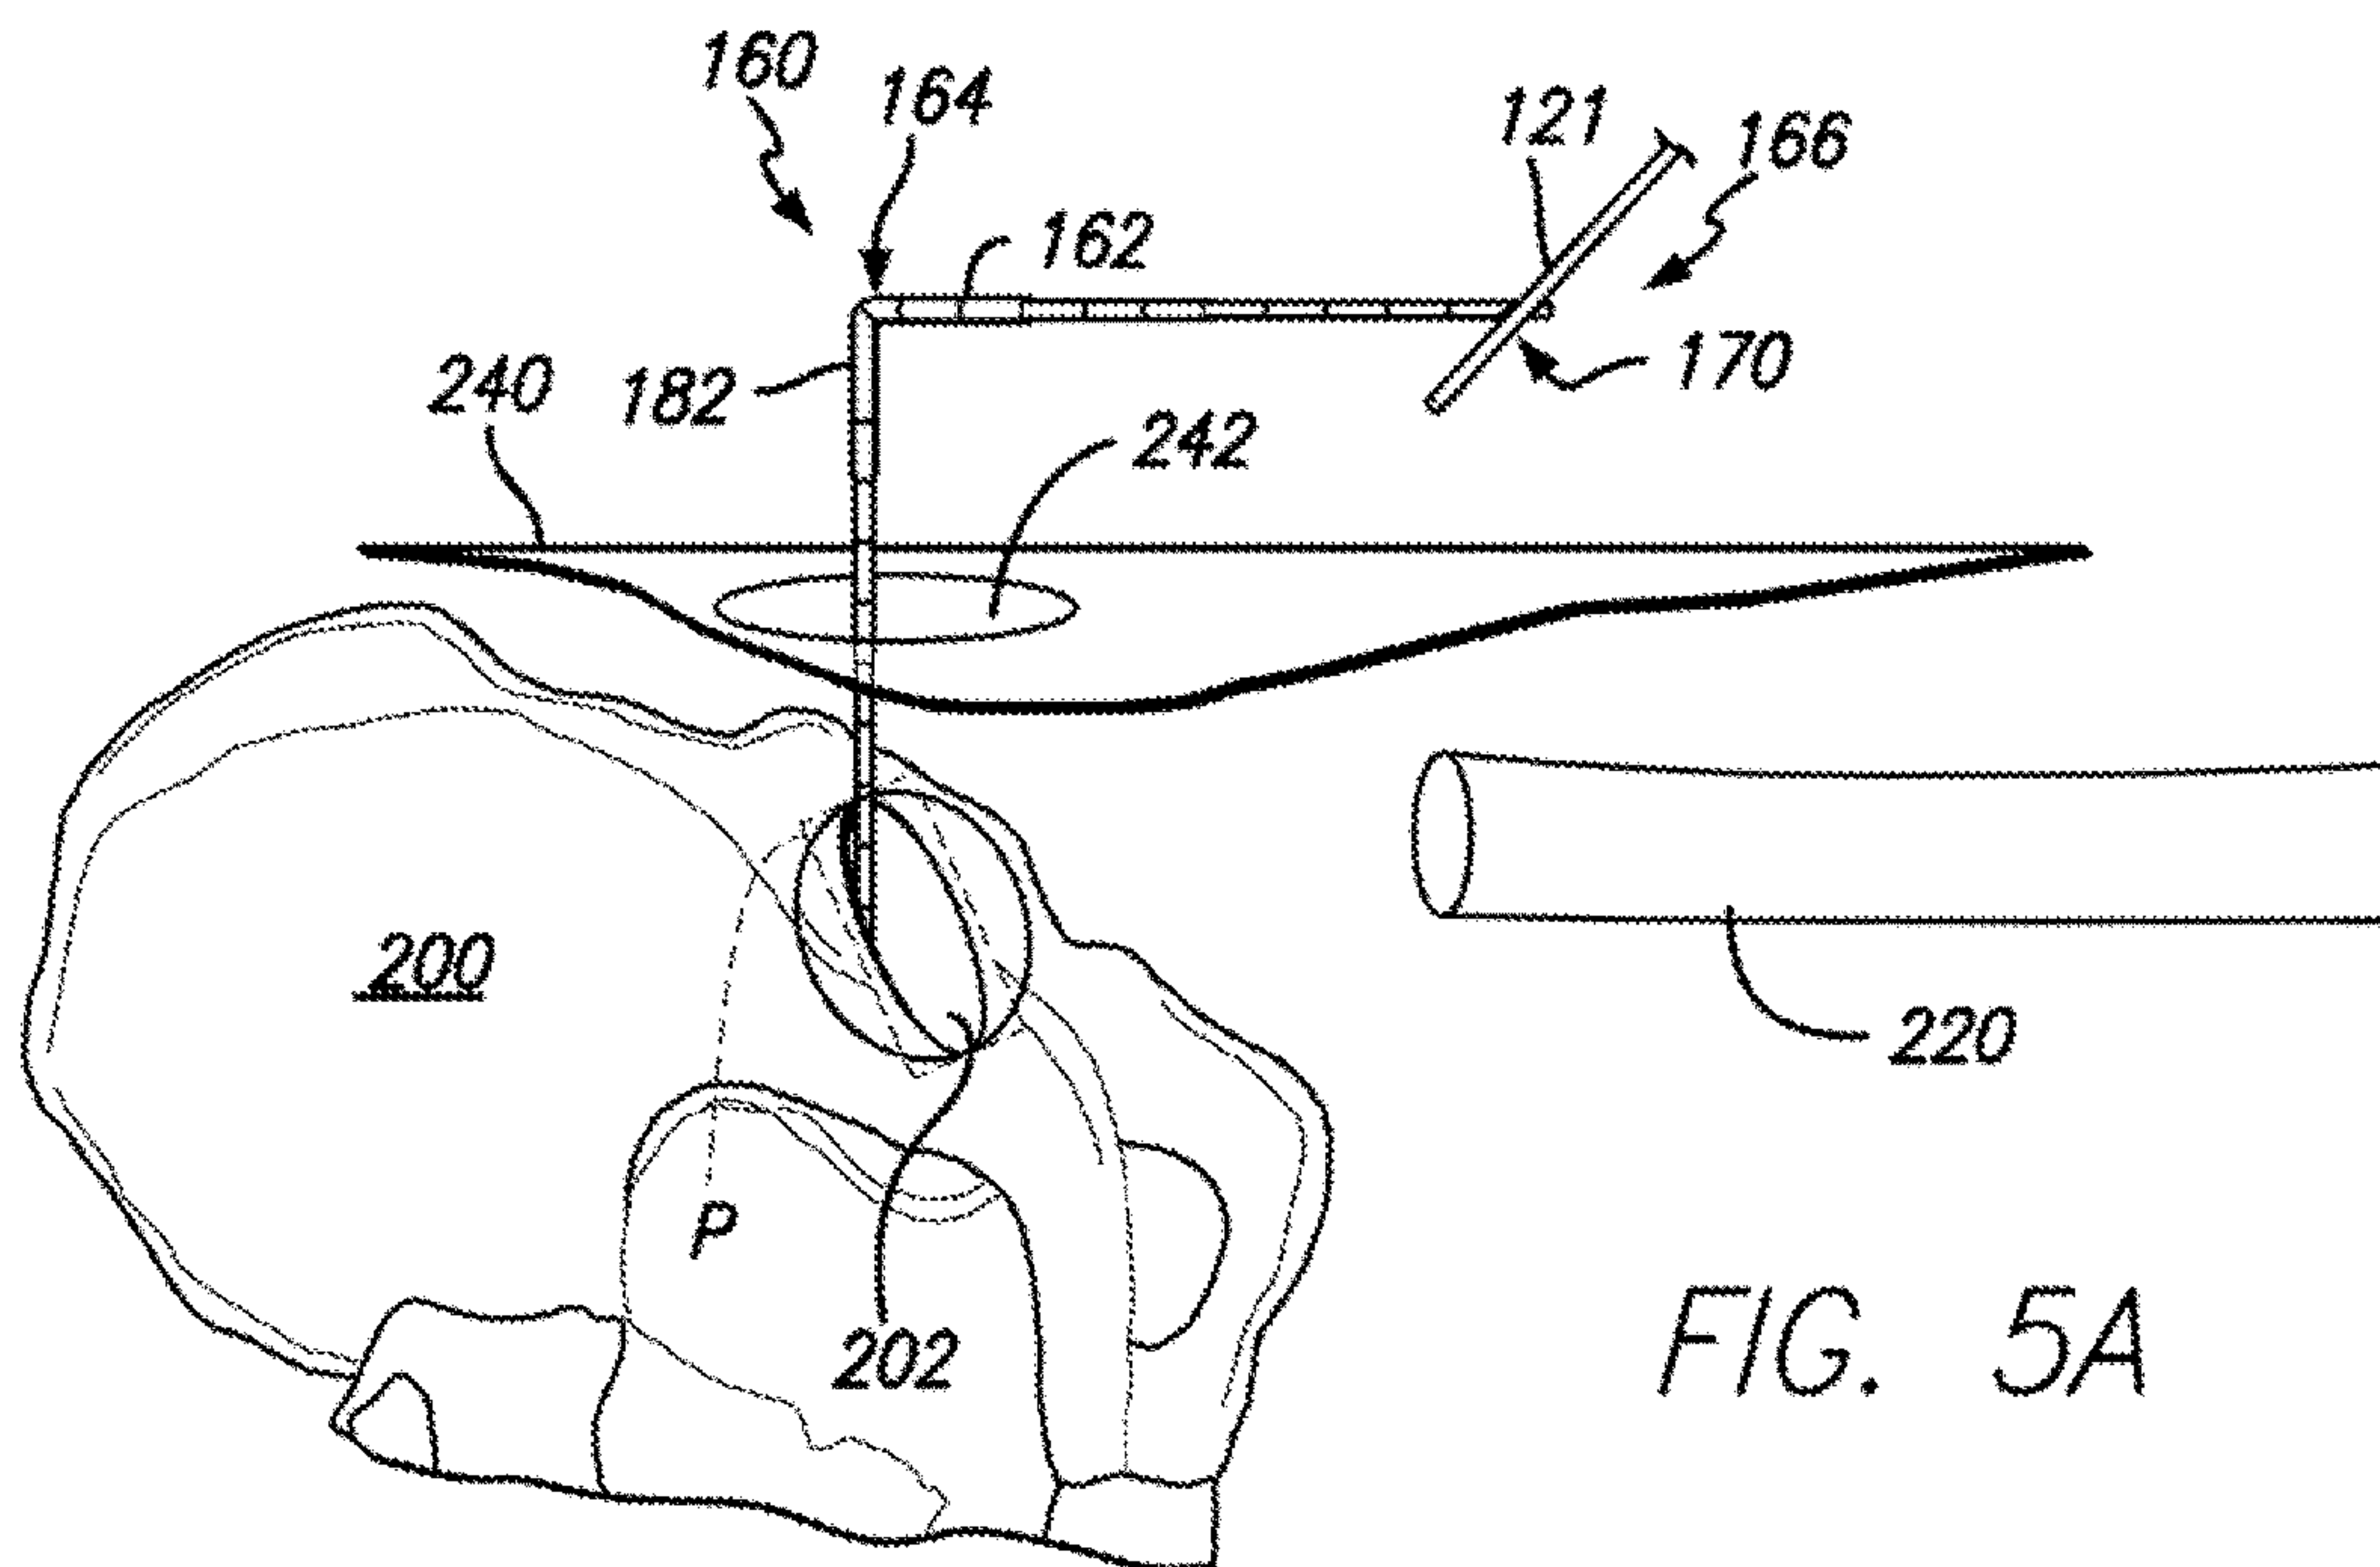


FIG. 4D





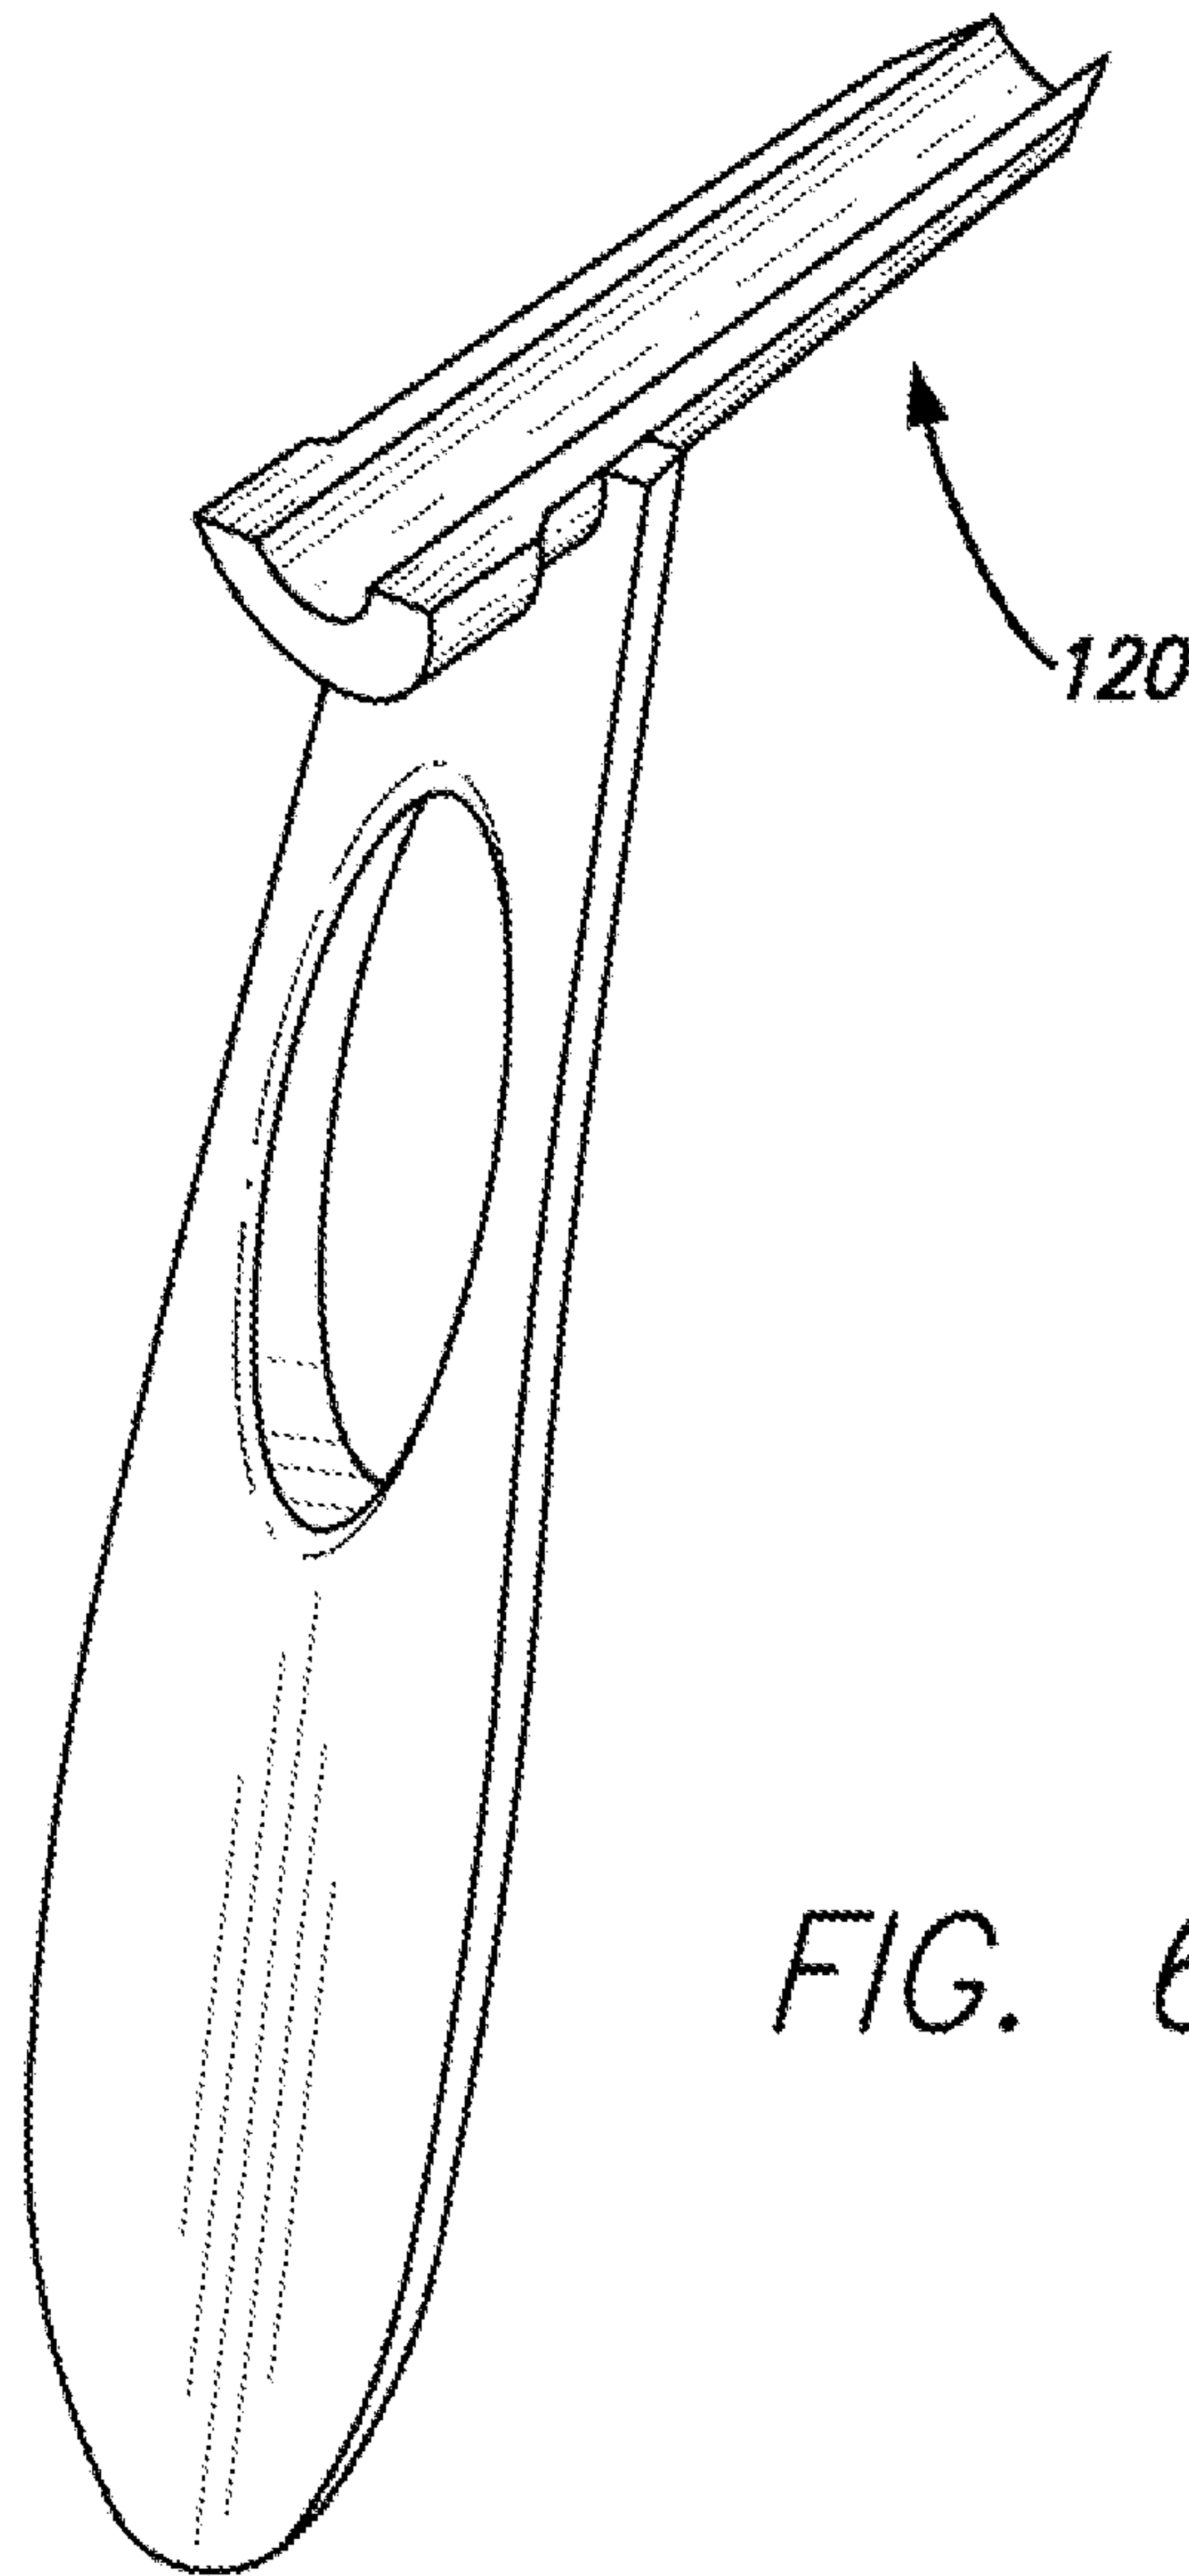


FIG. 6



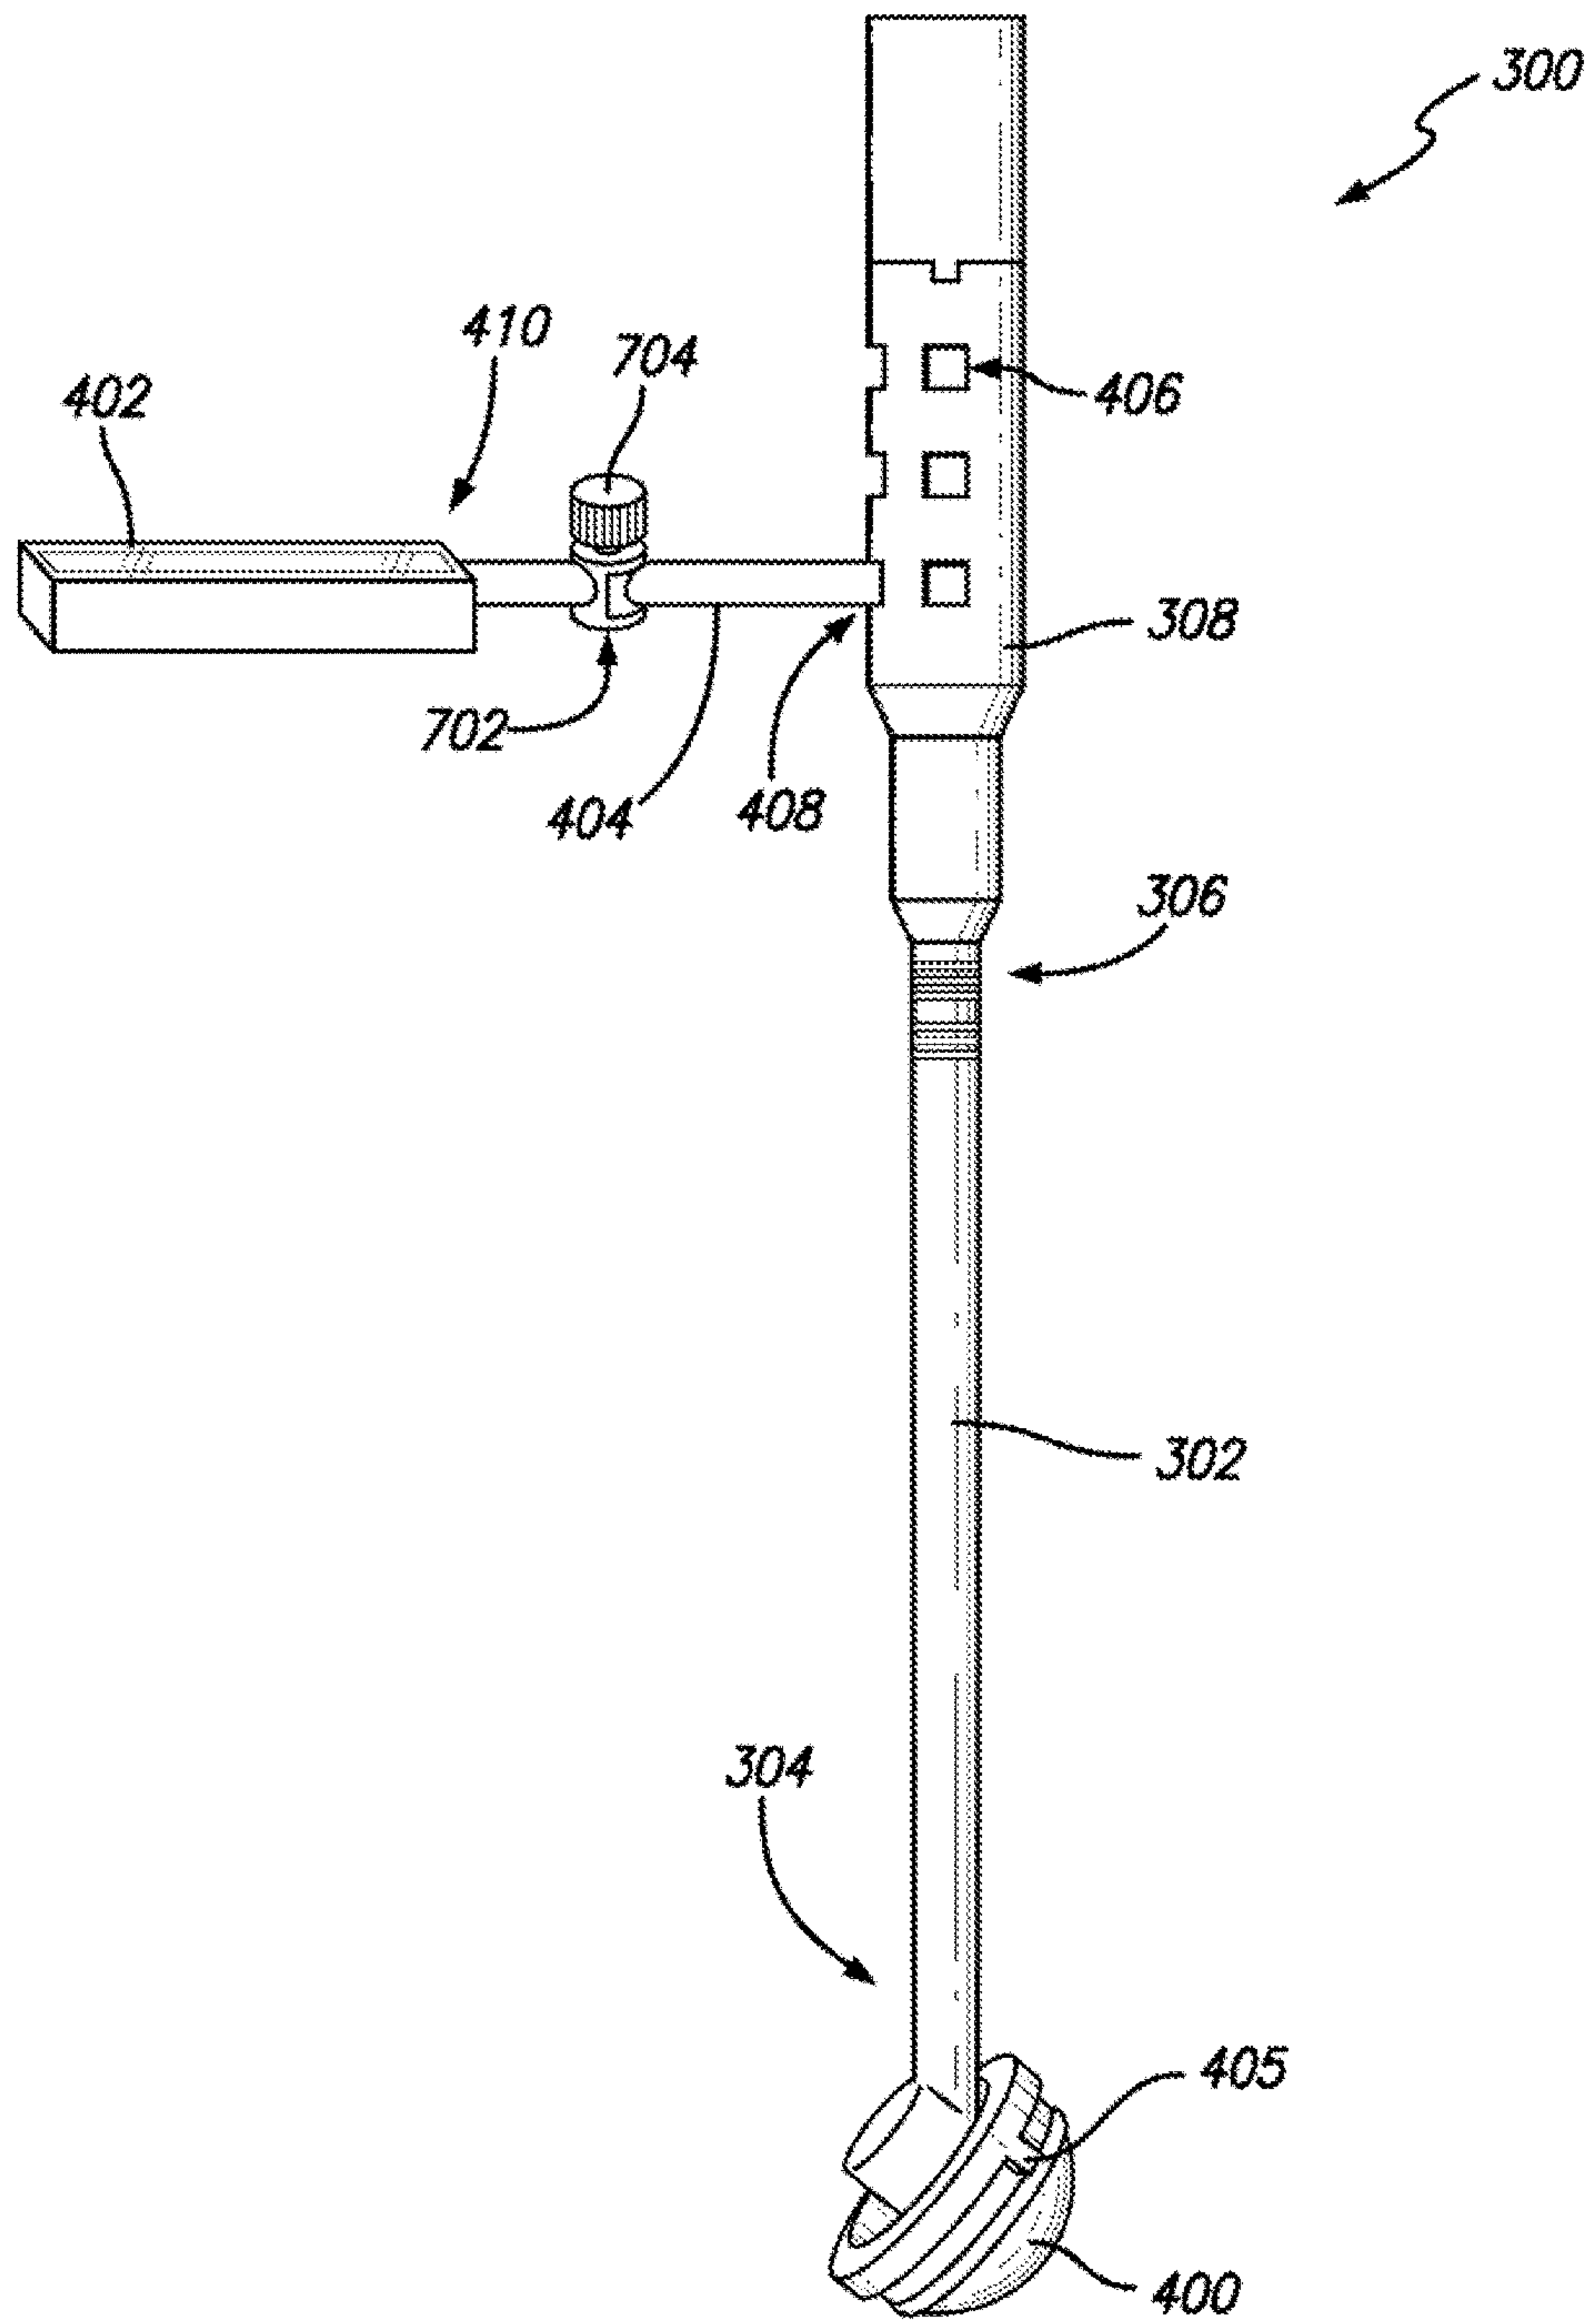


FIG. 7A

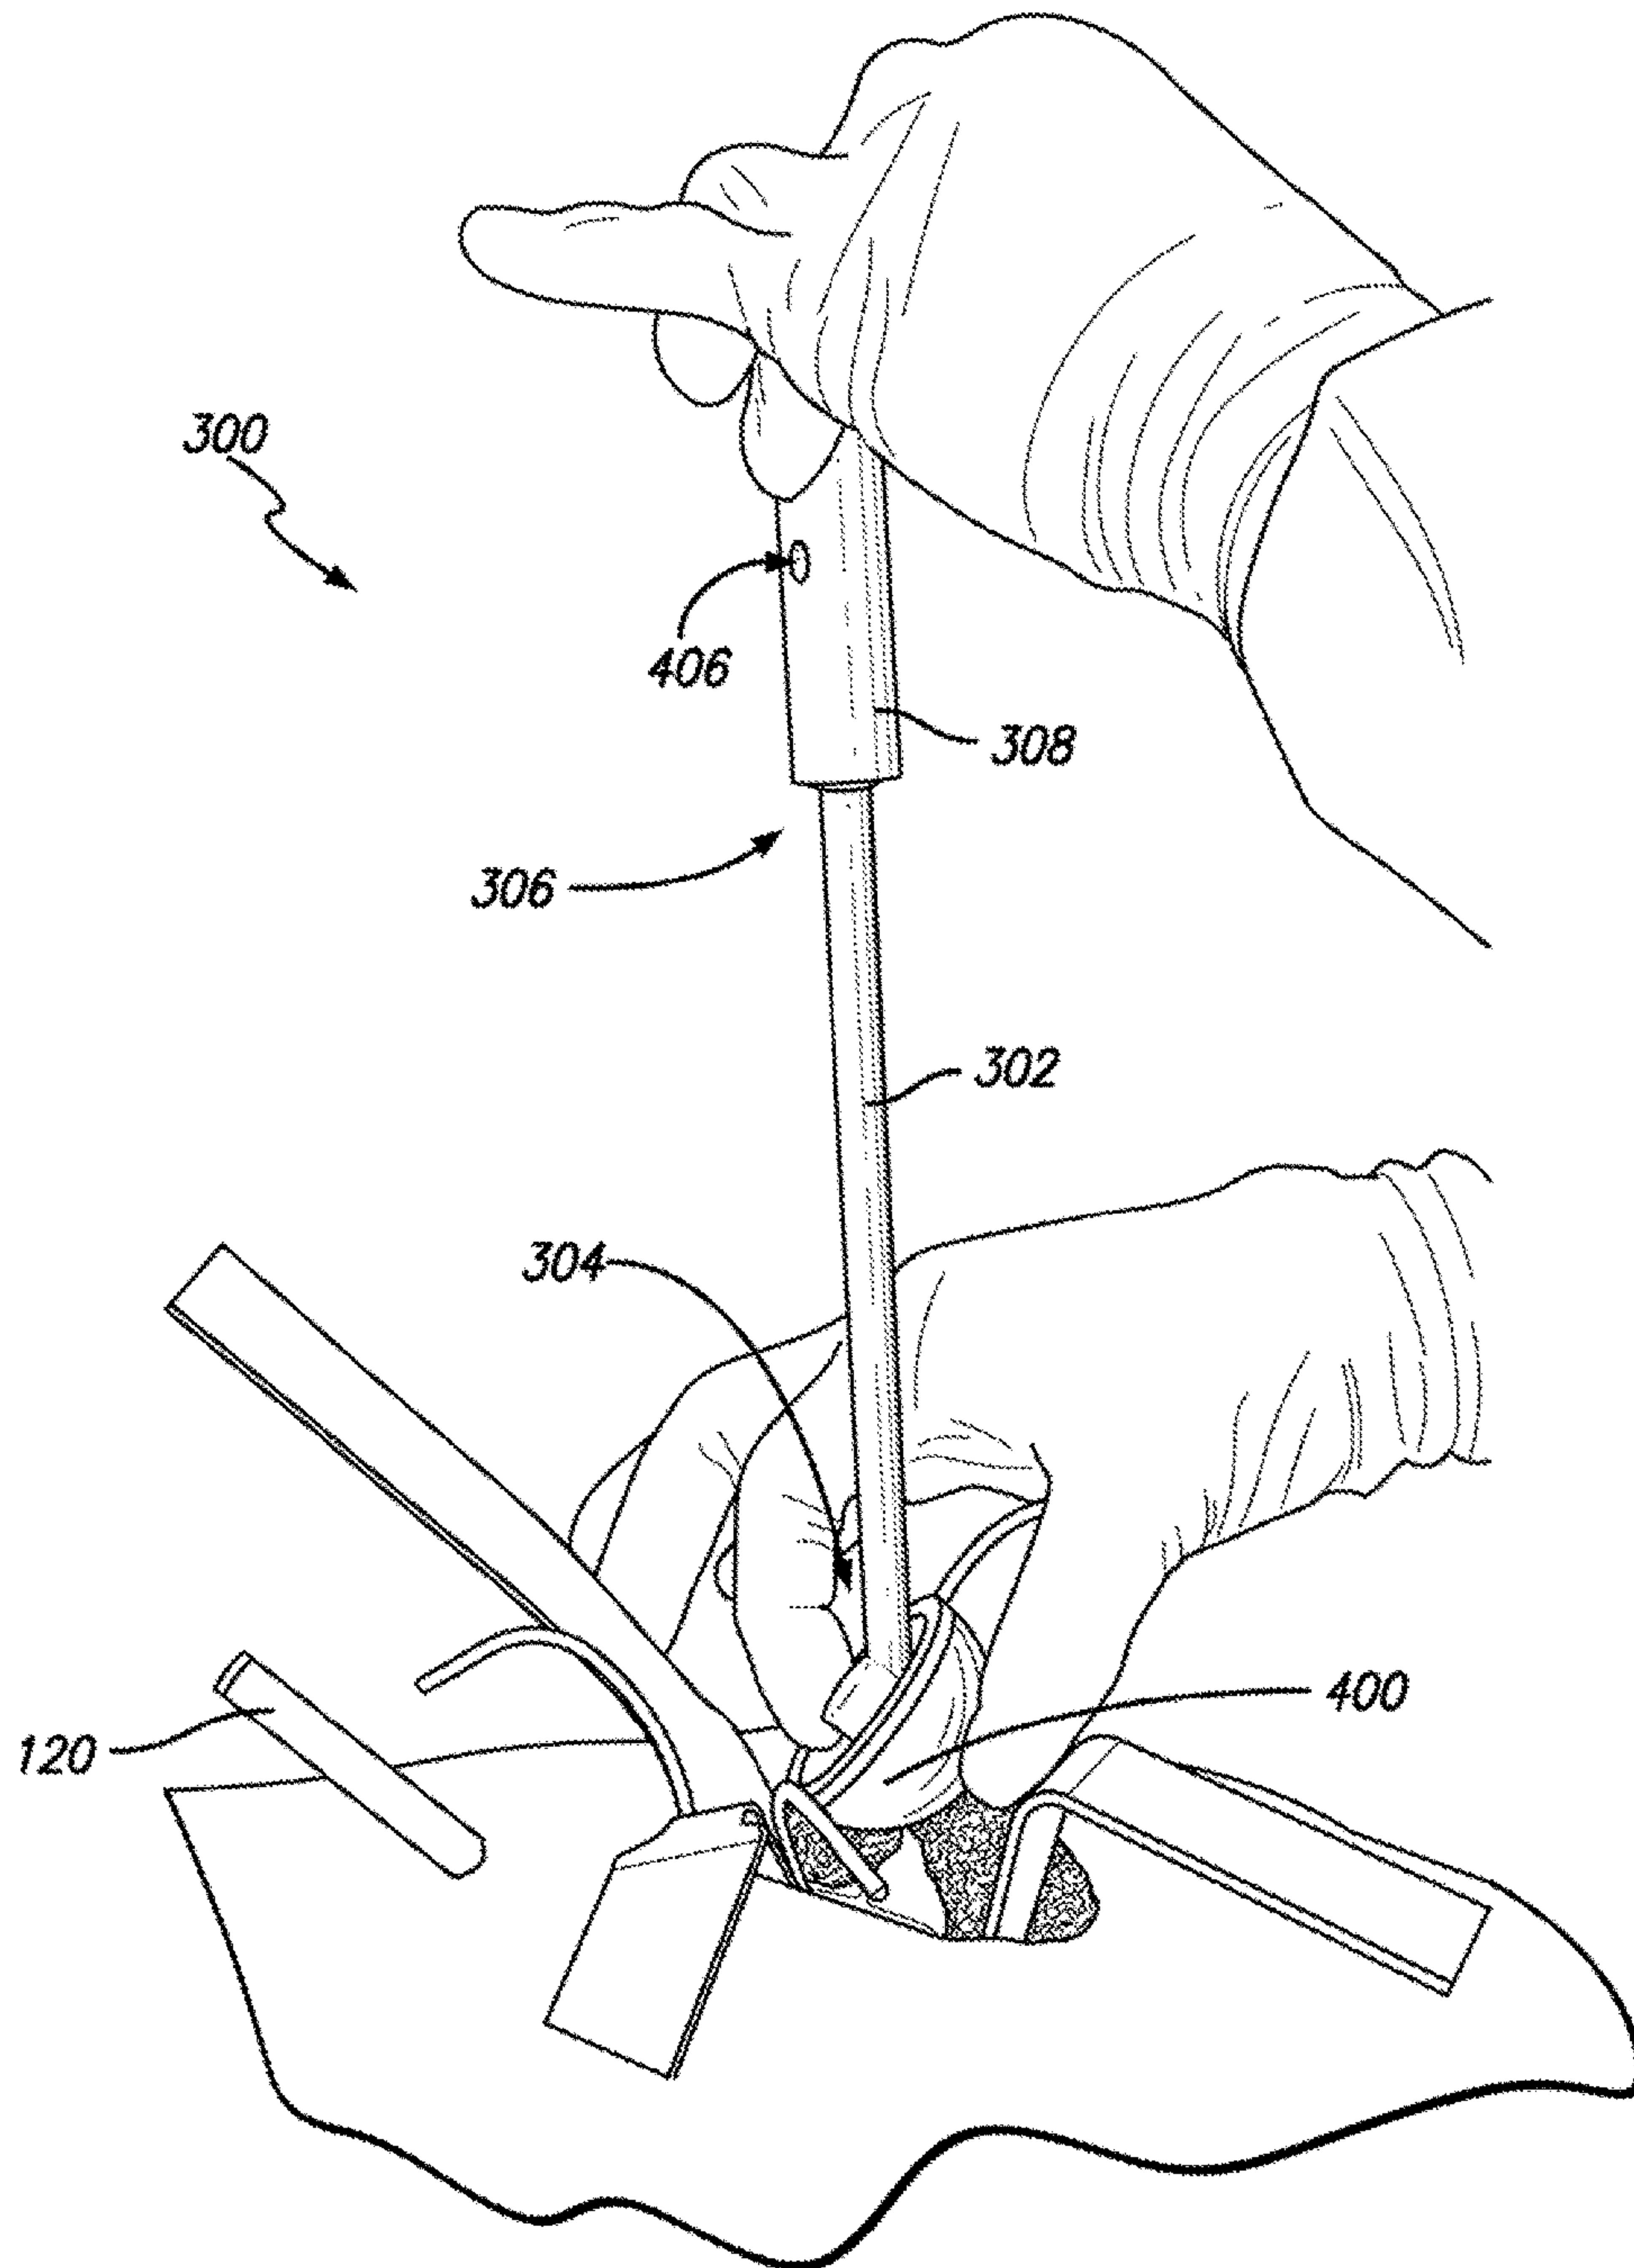


FIG. 7B

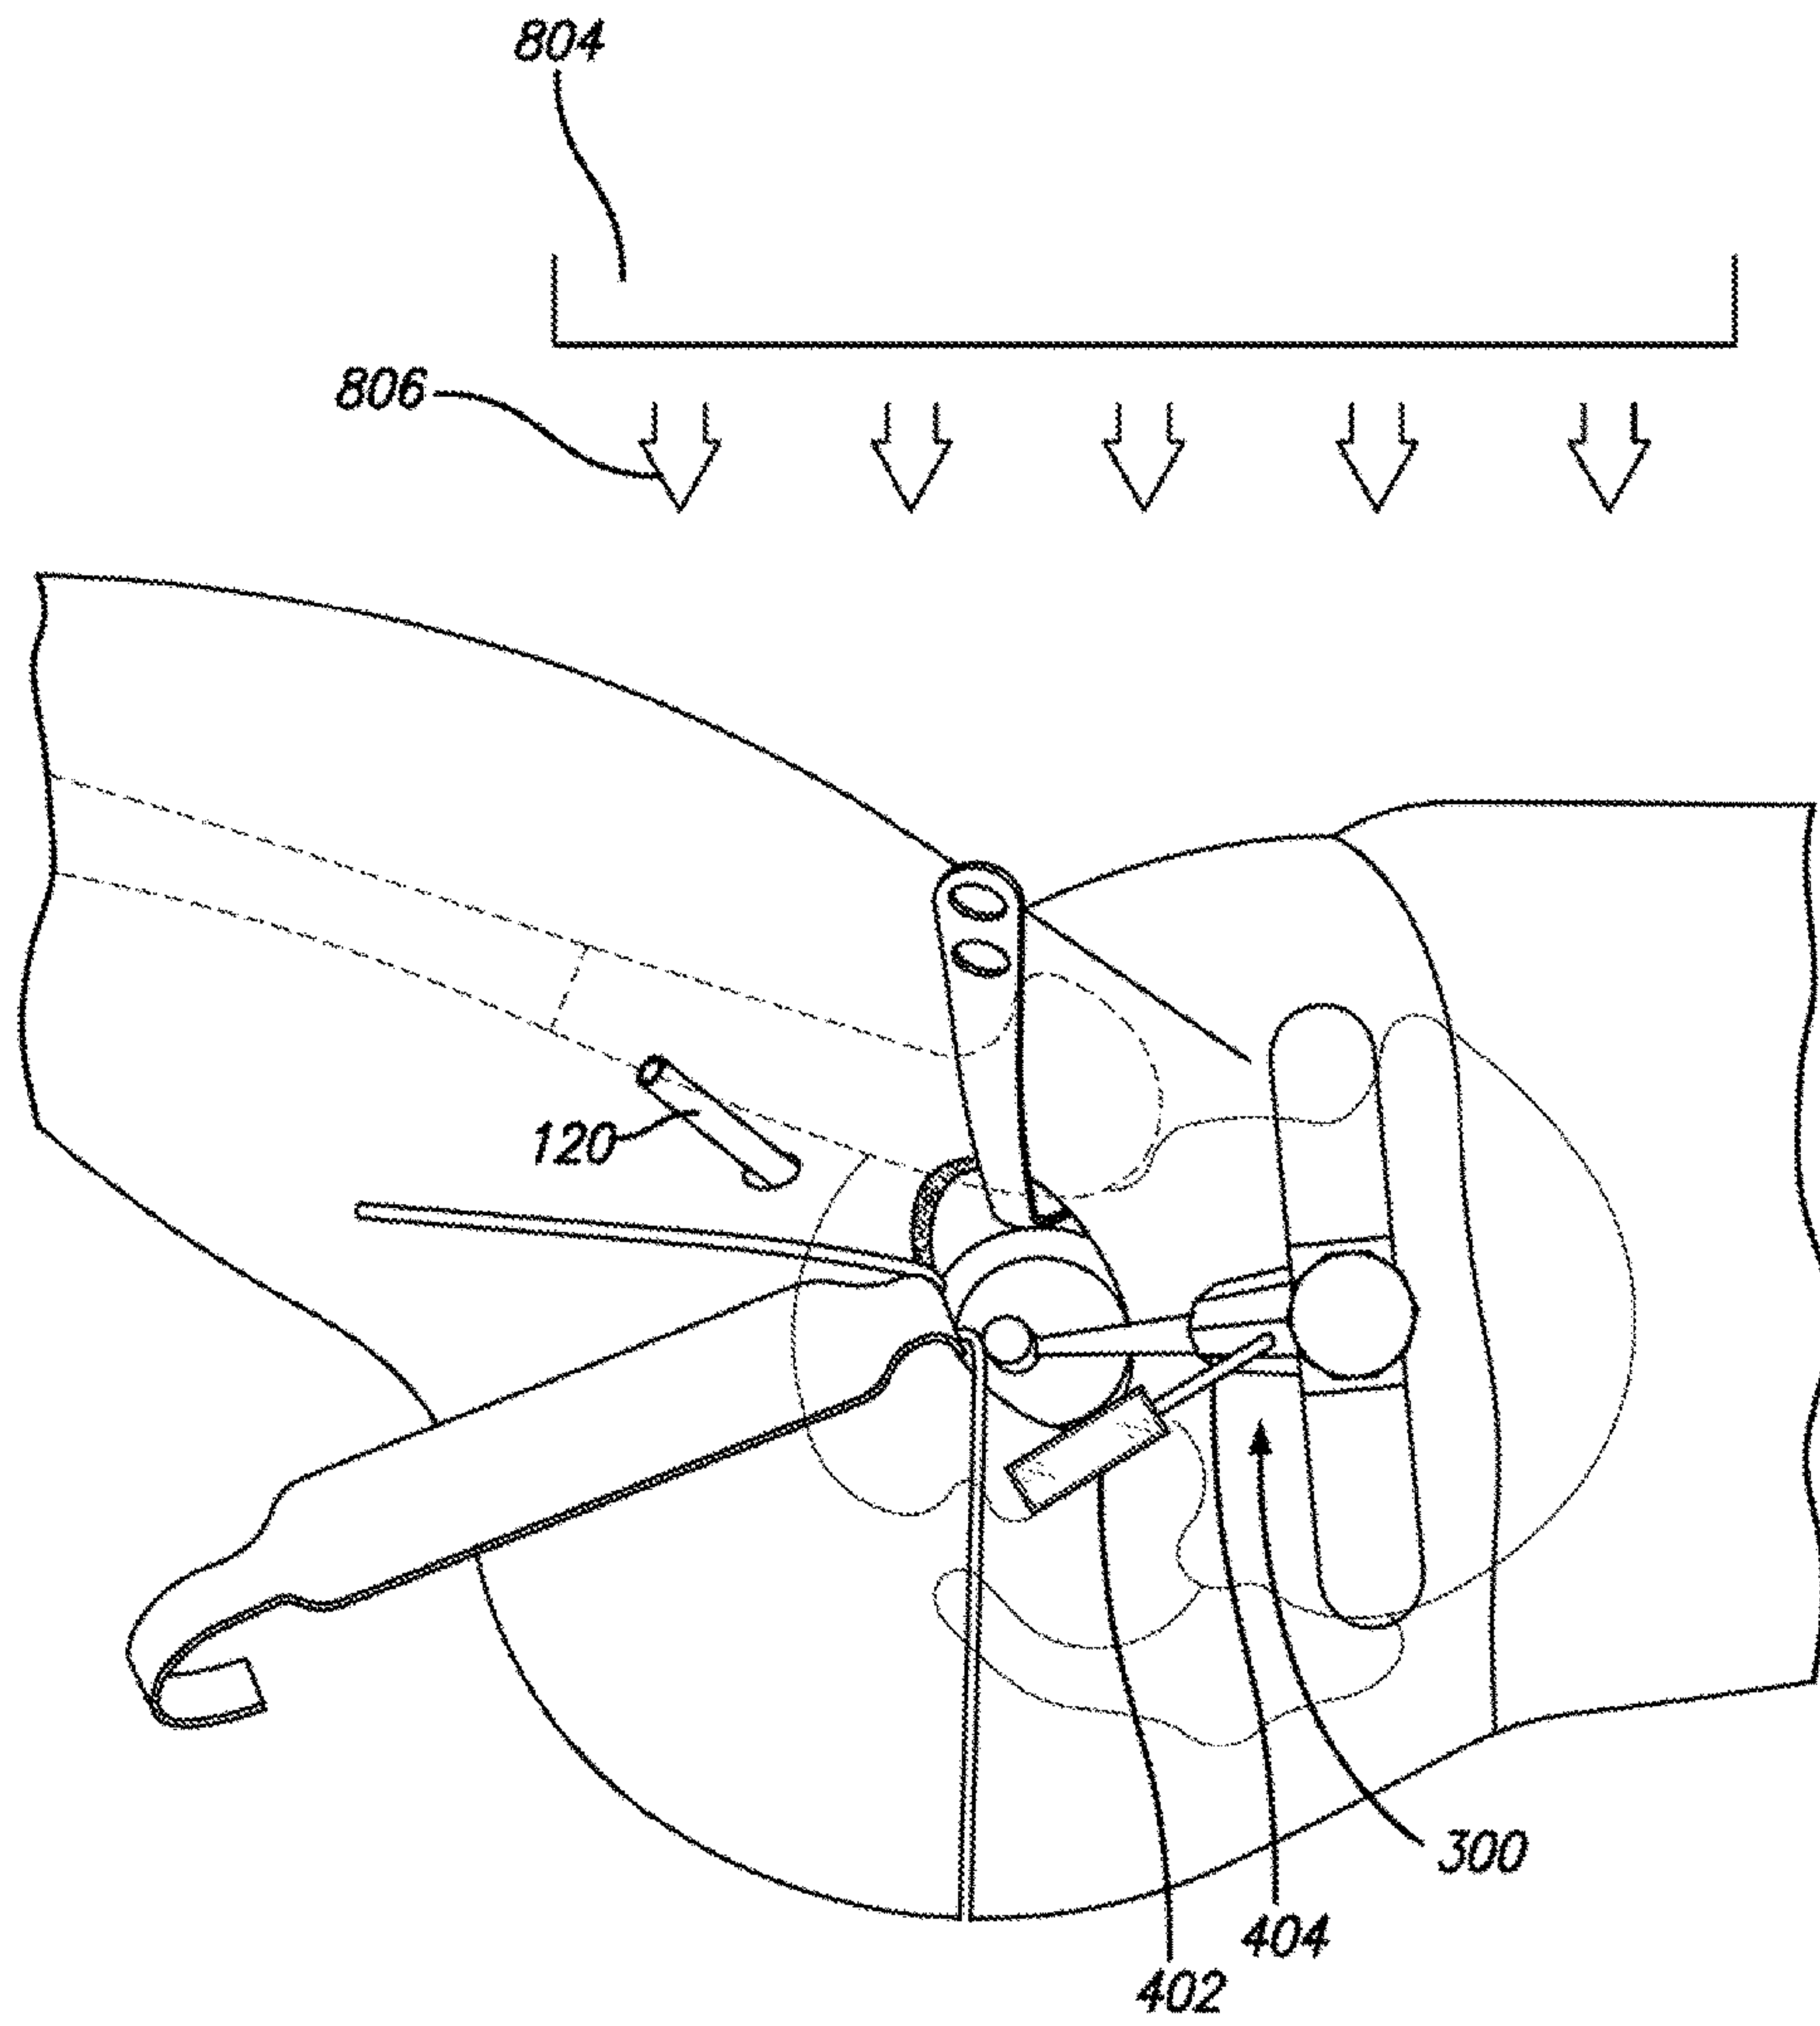


FIG. 8



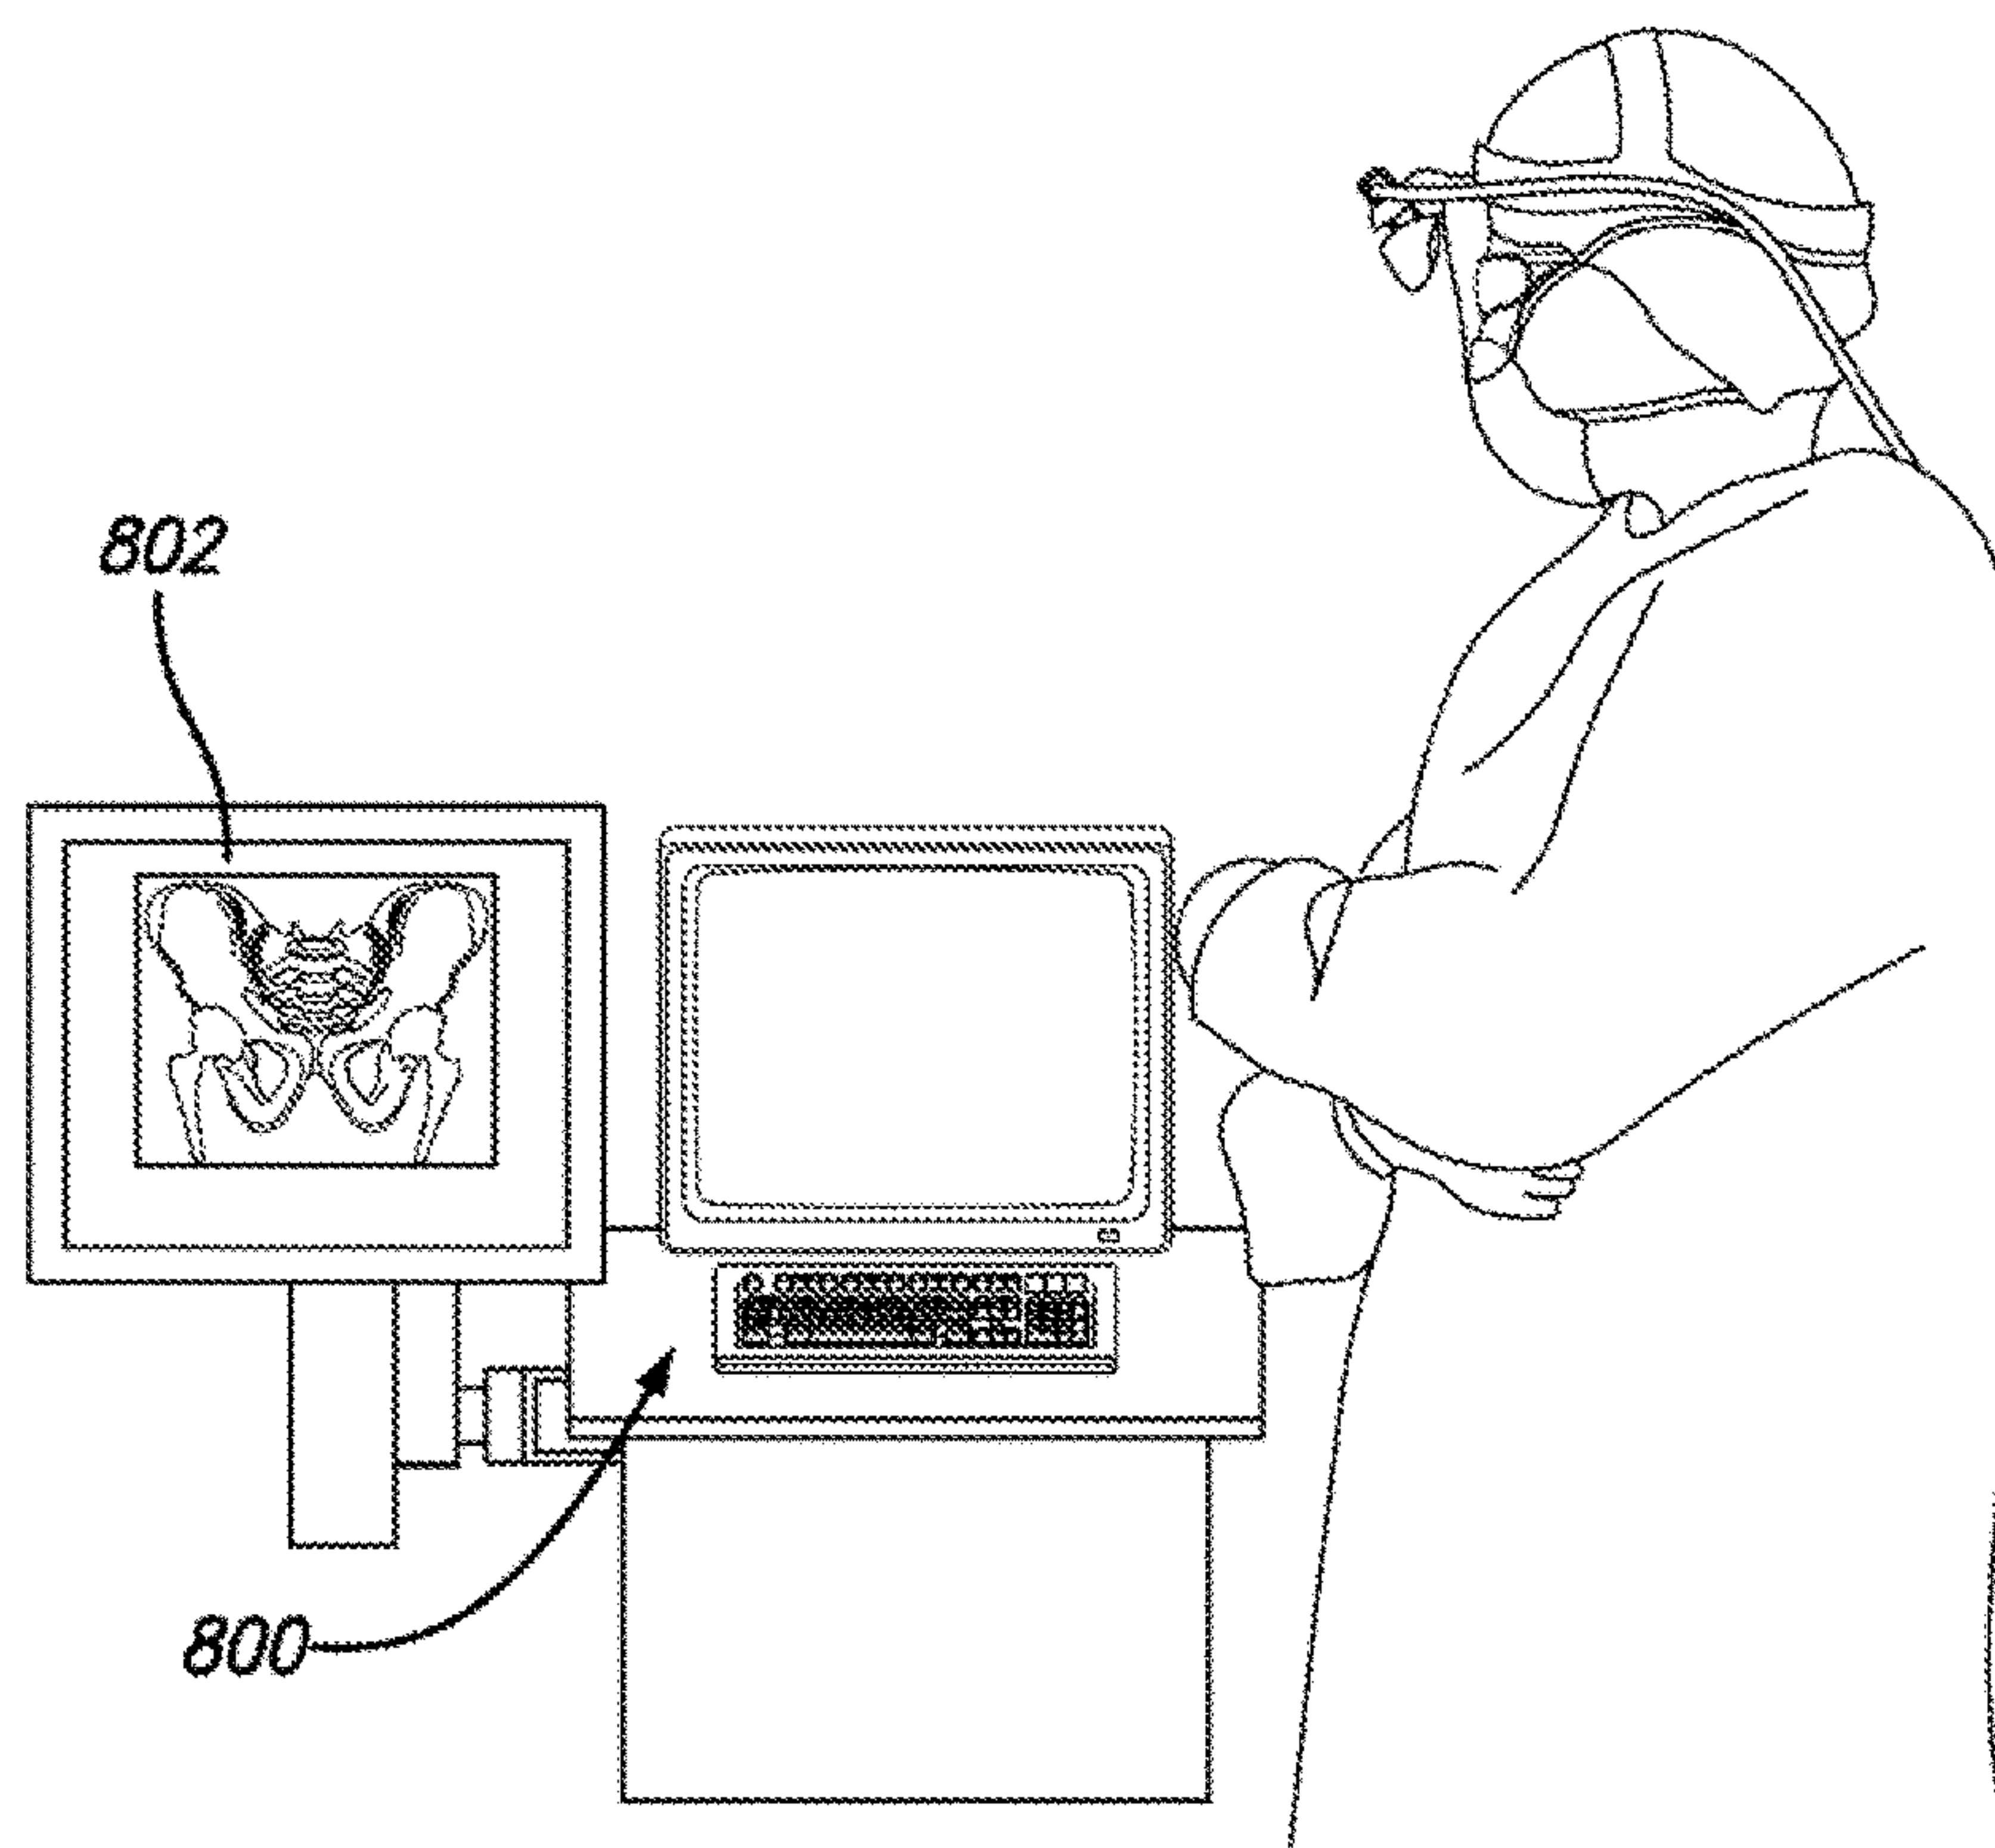


FIG. 9

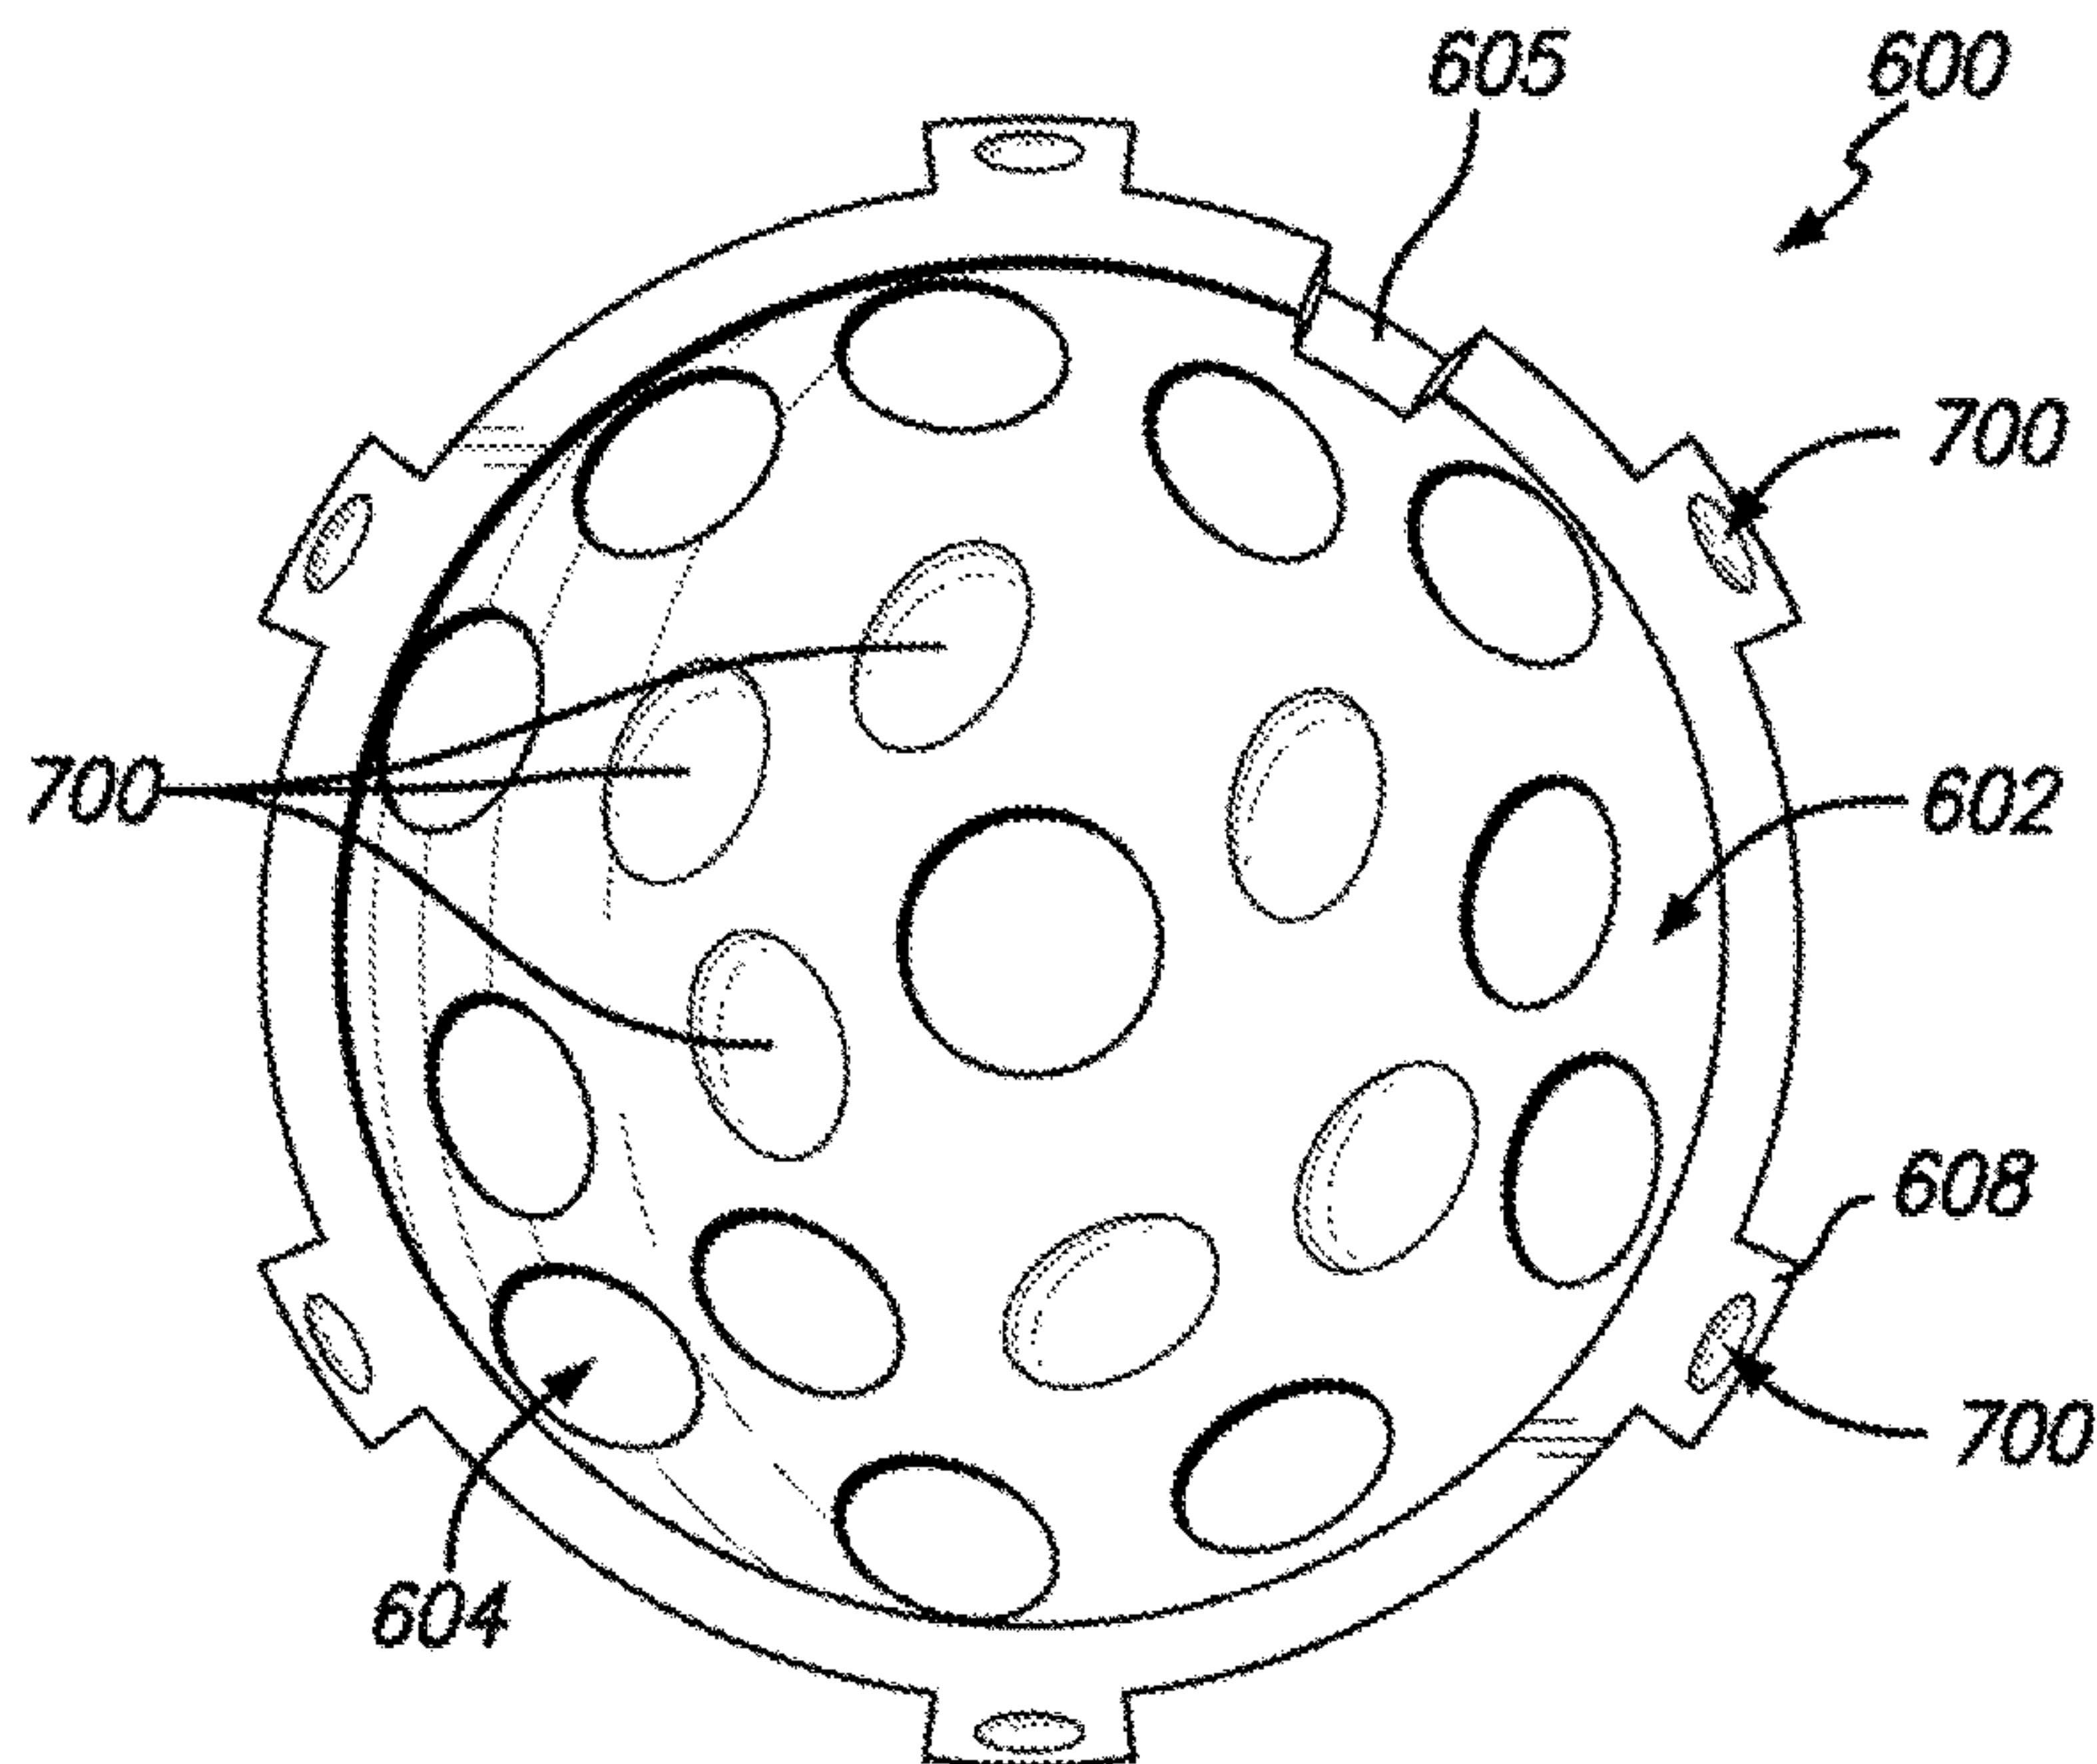
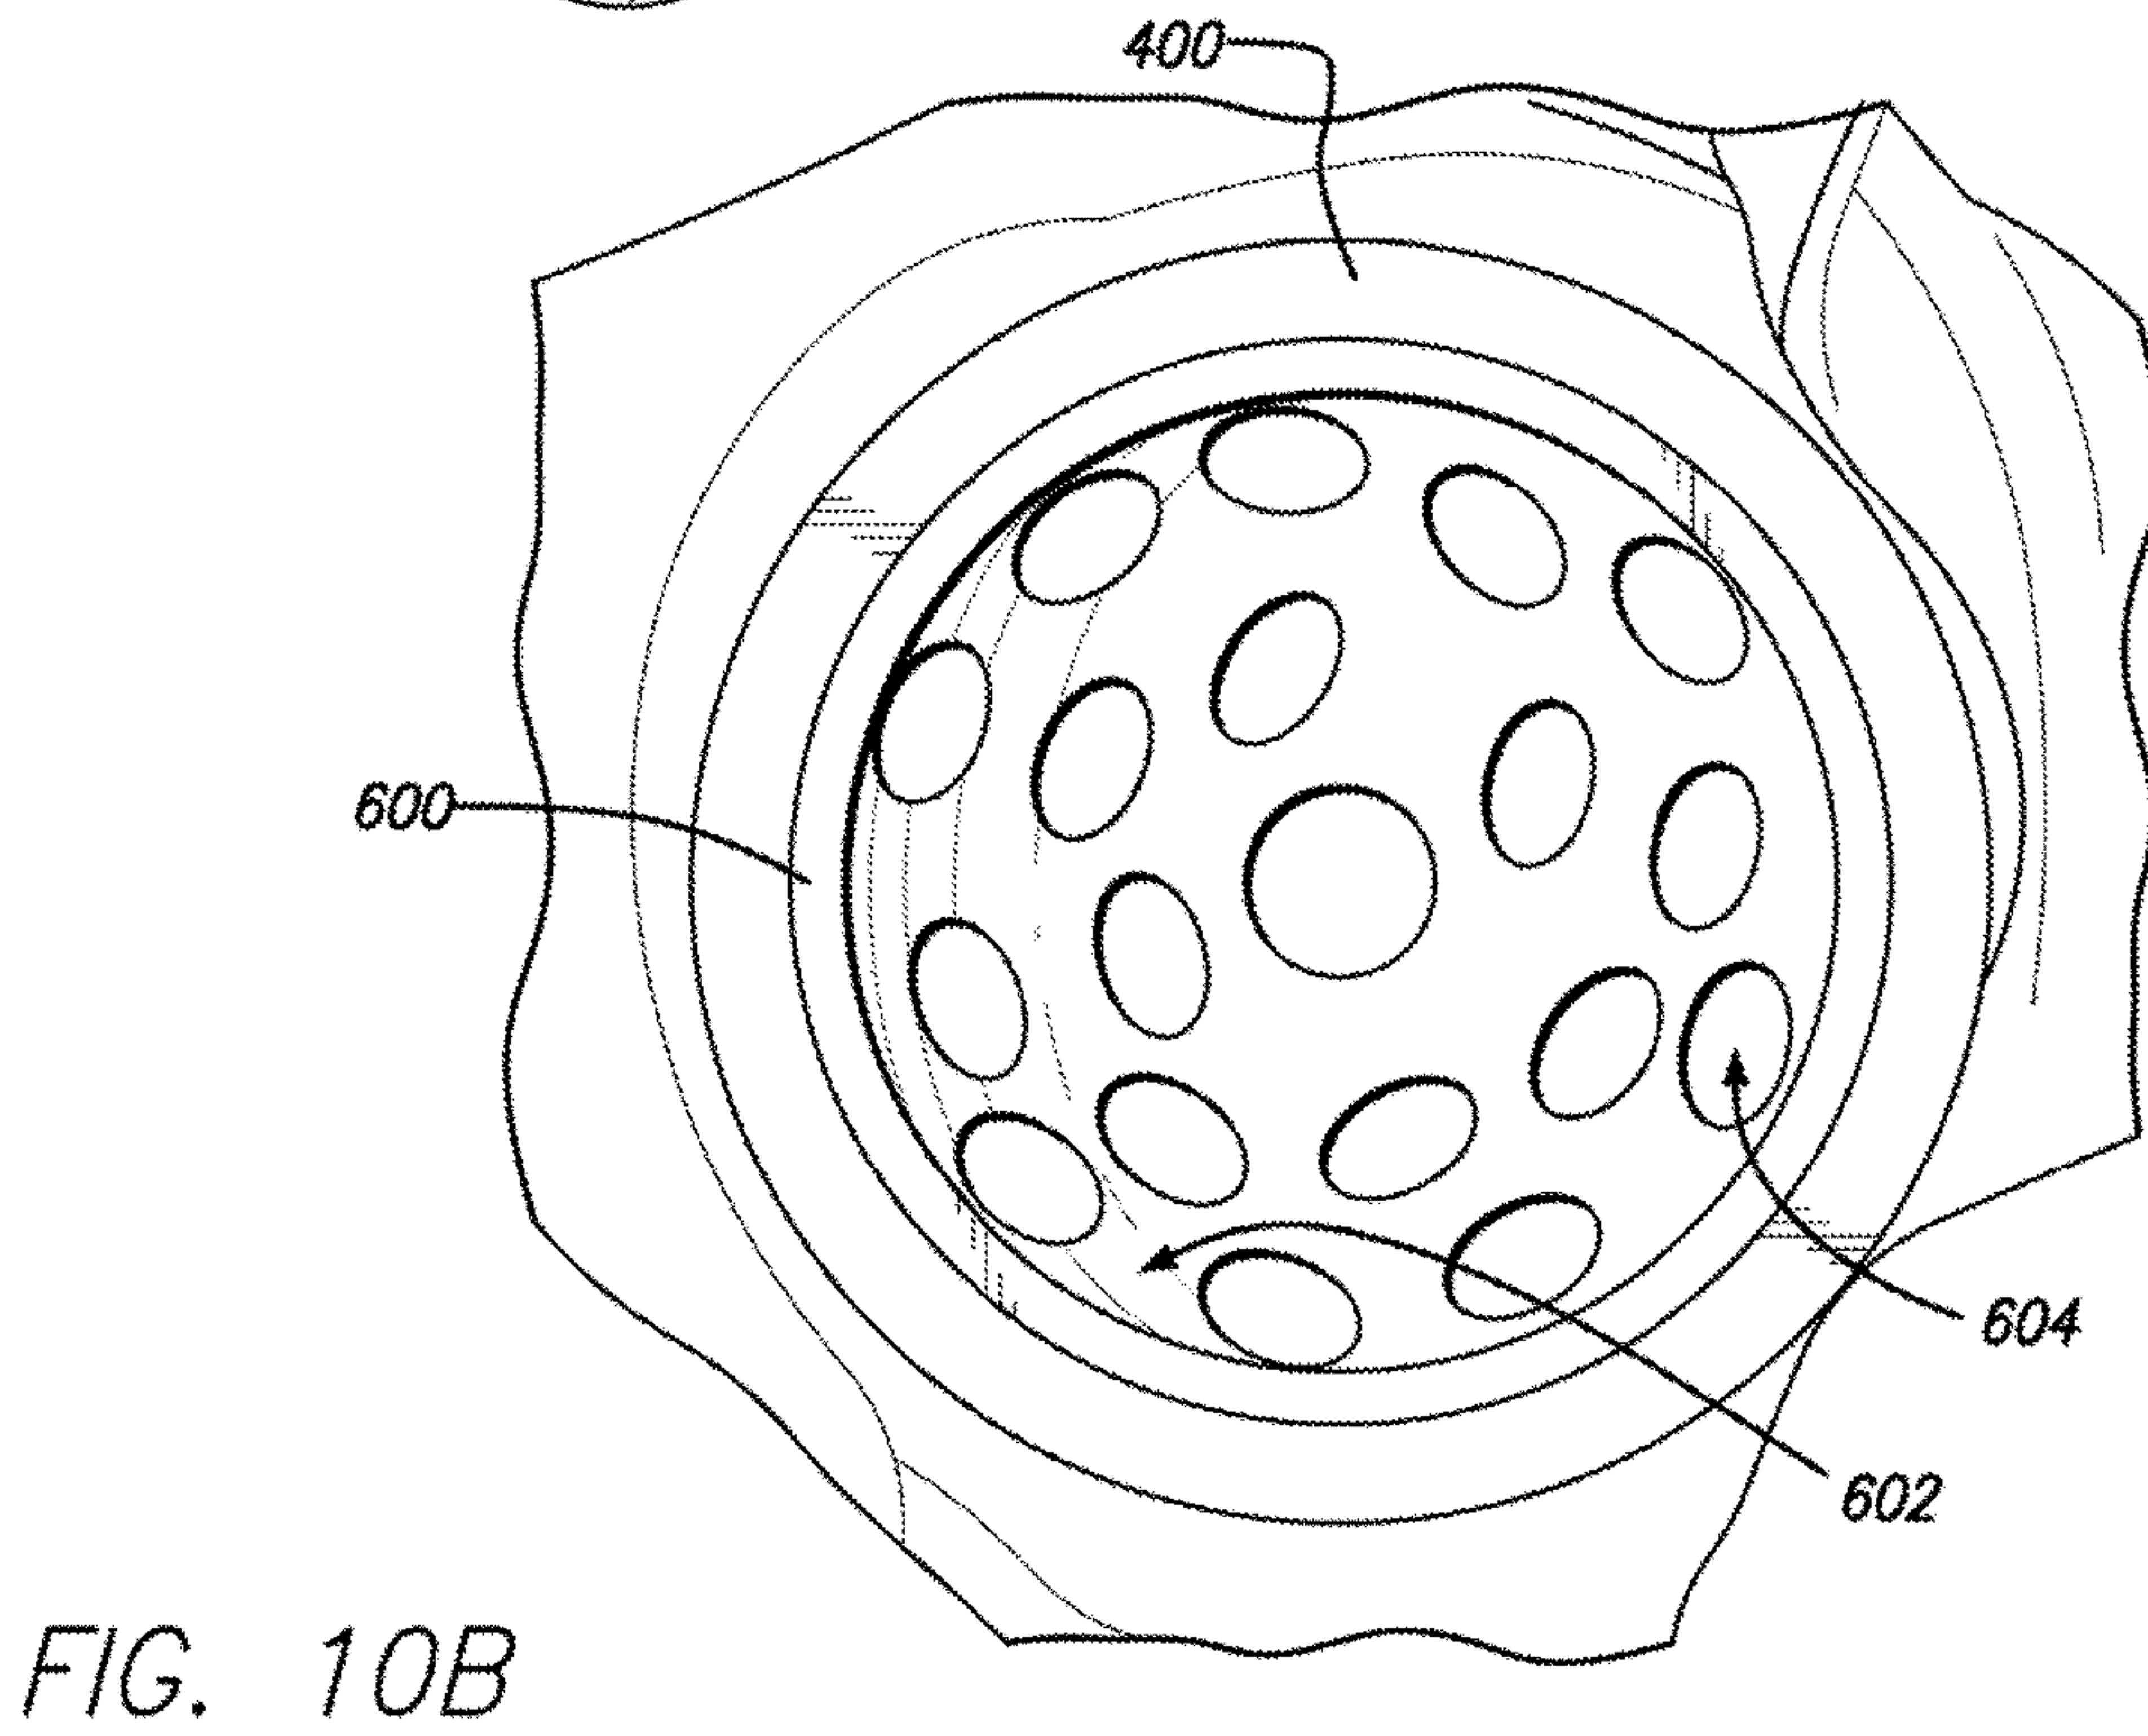
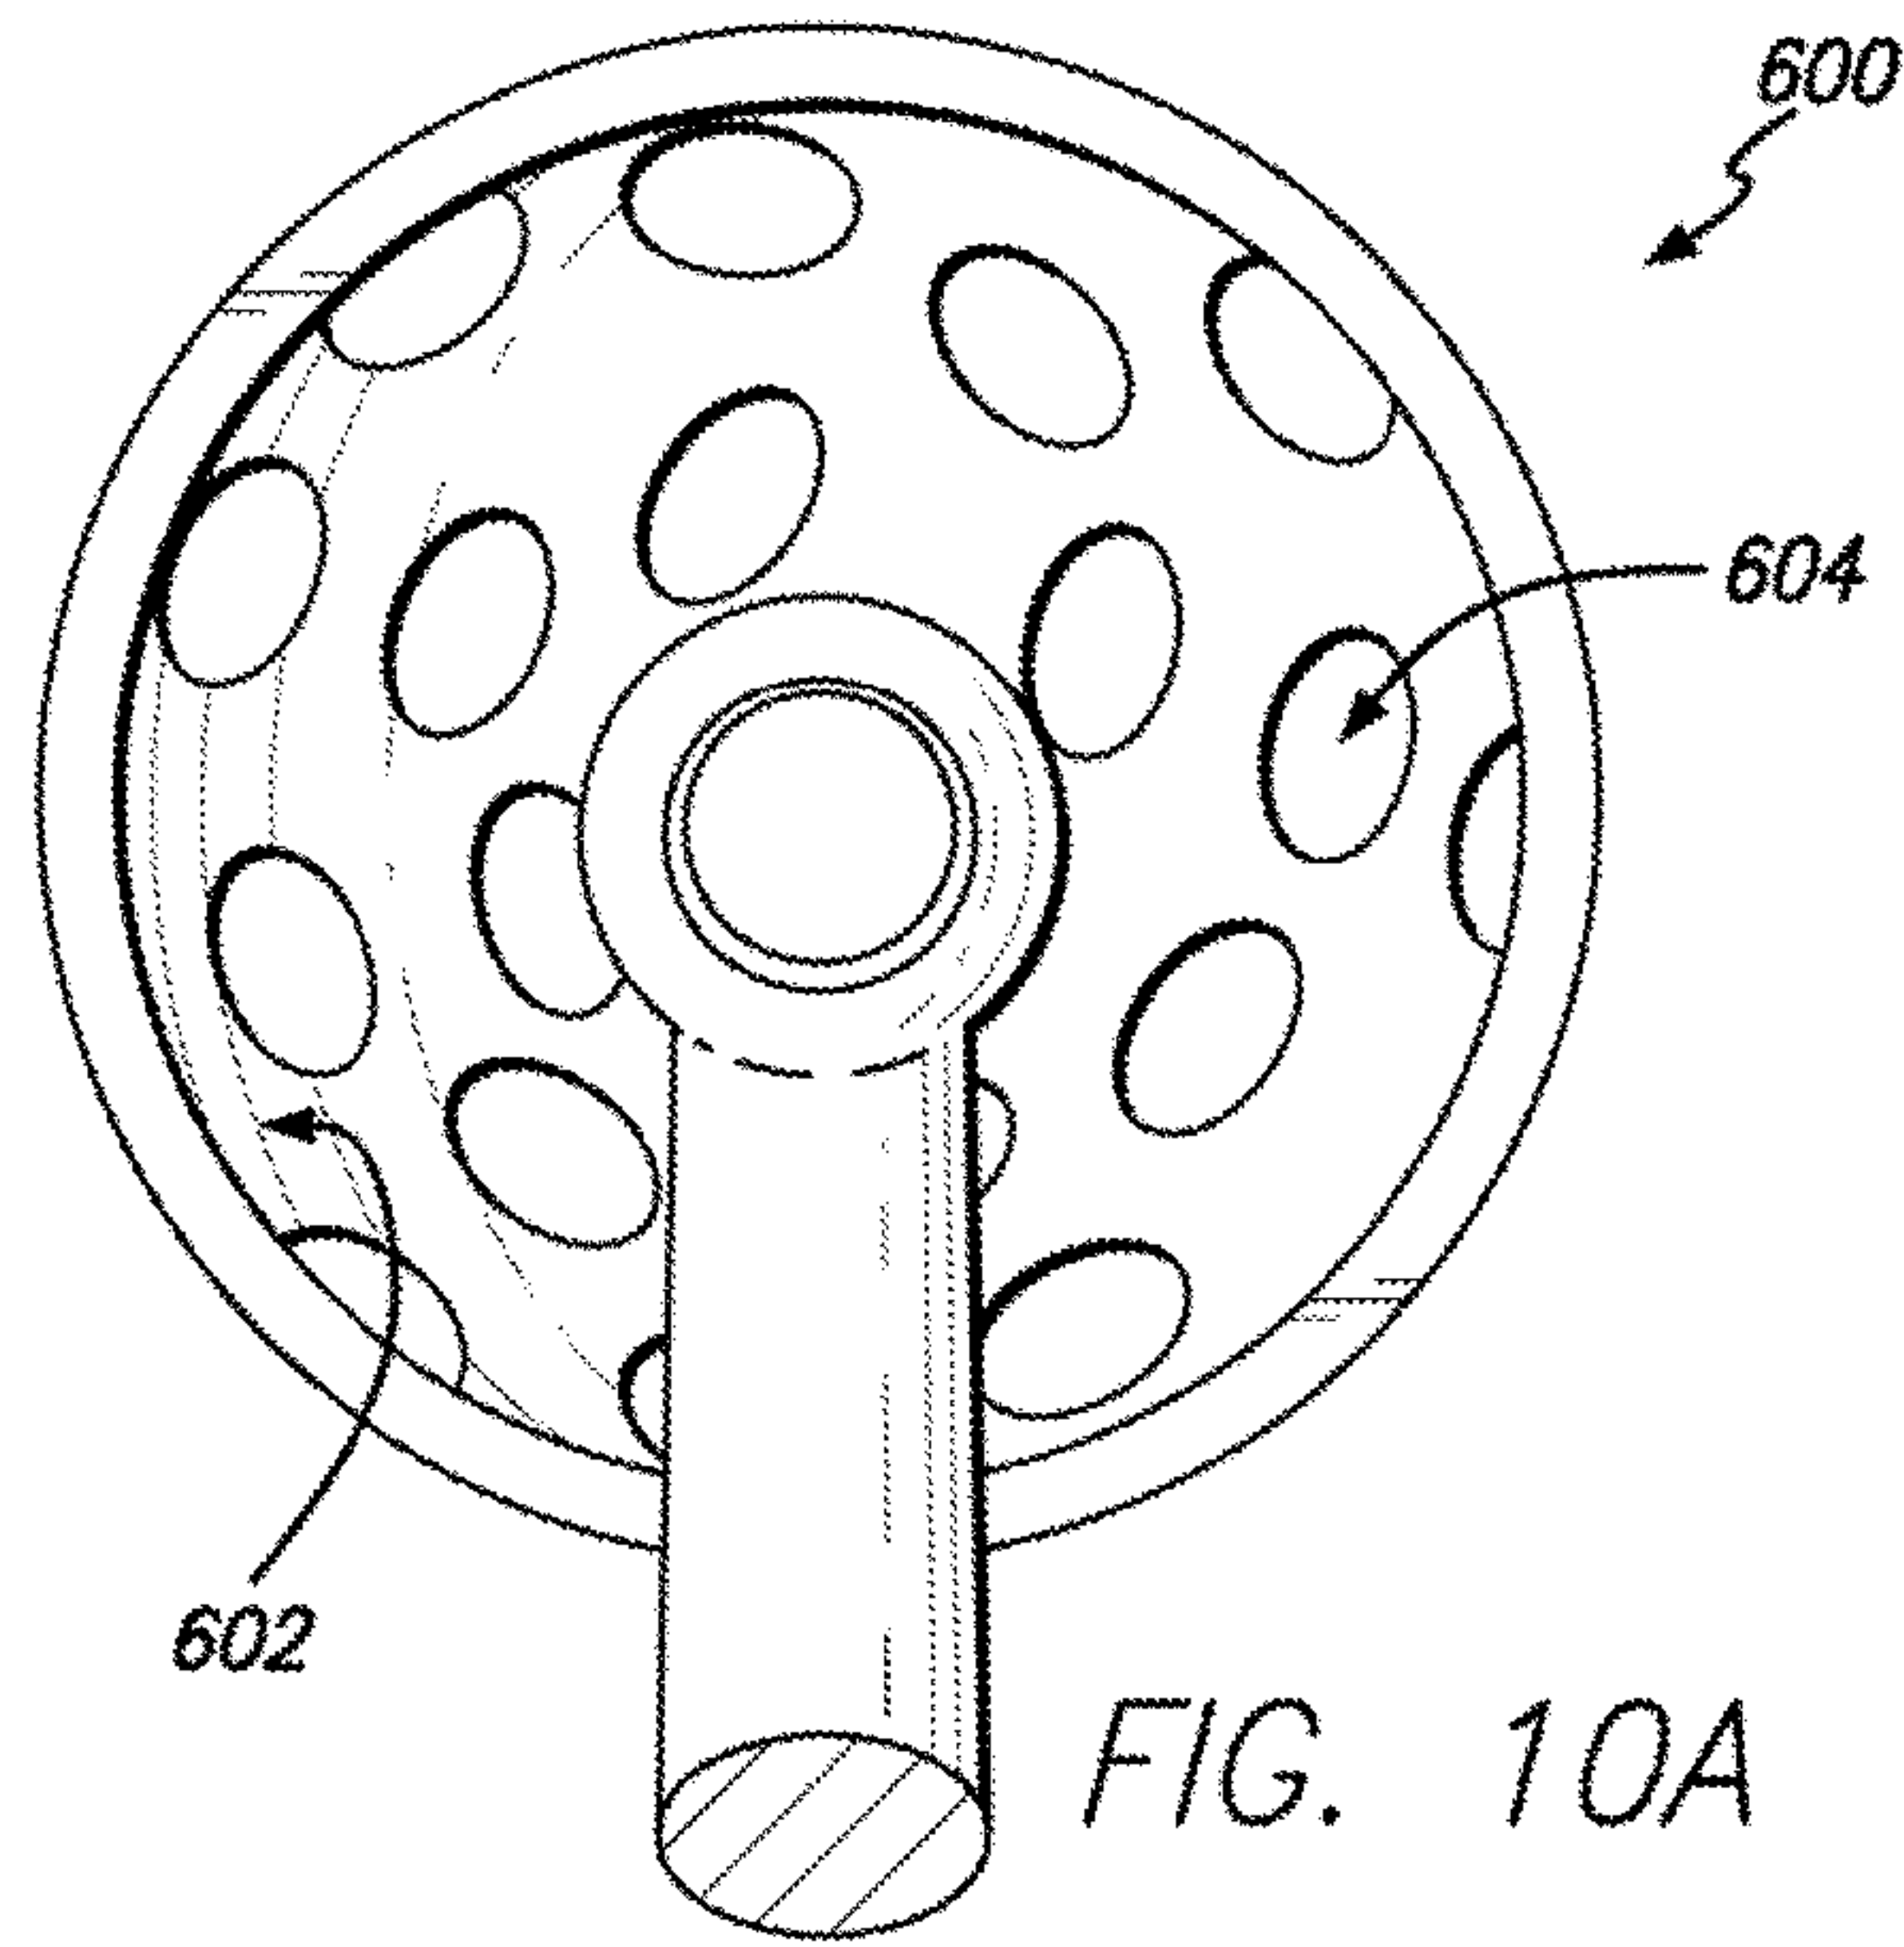


FIG. 11



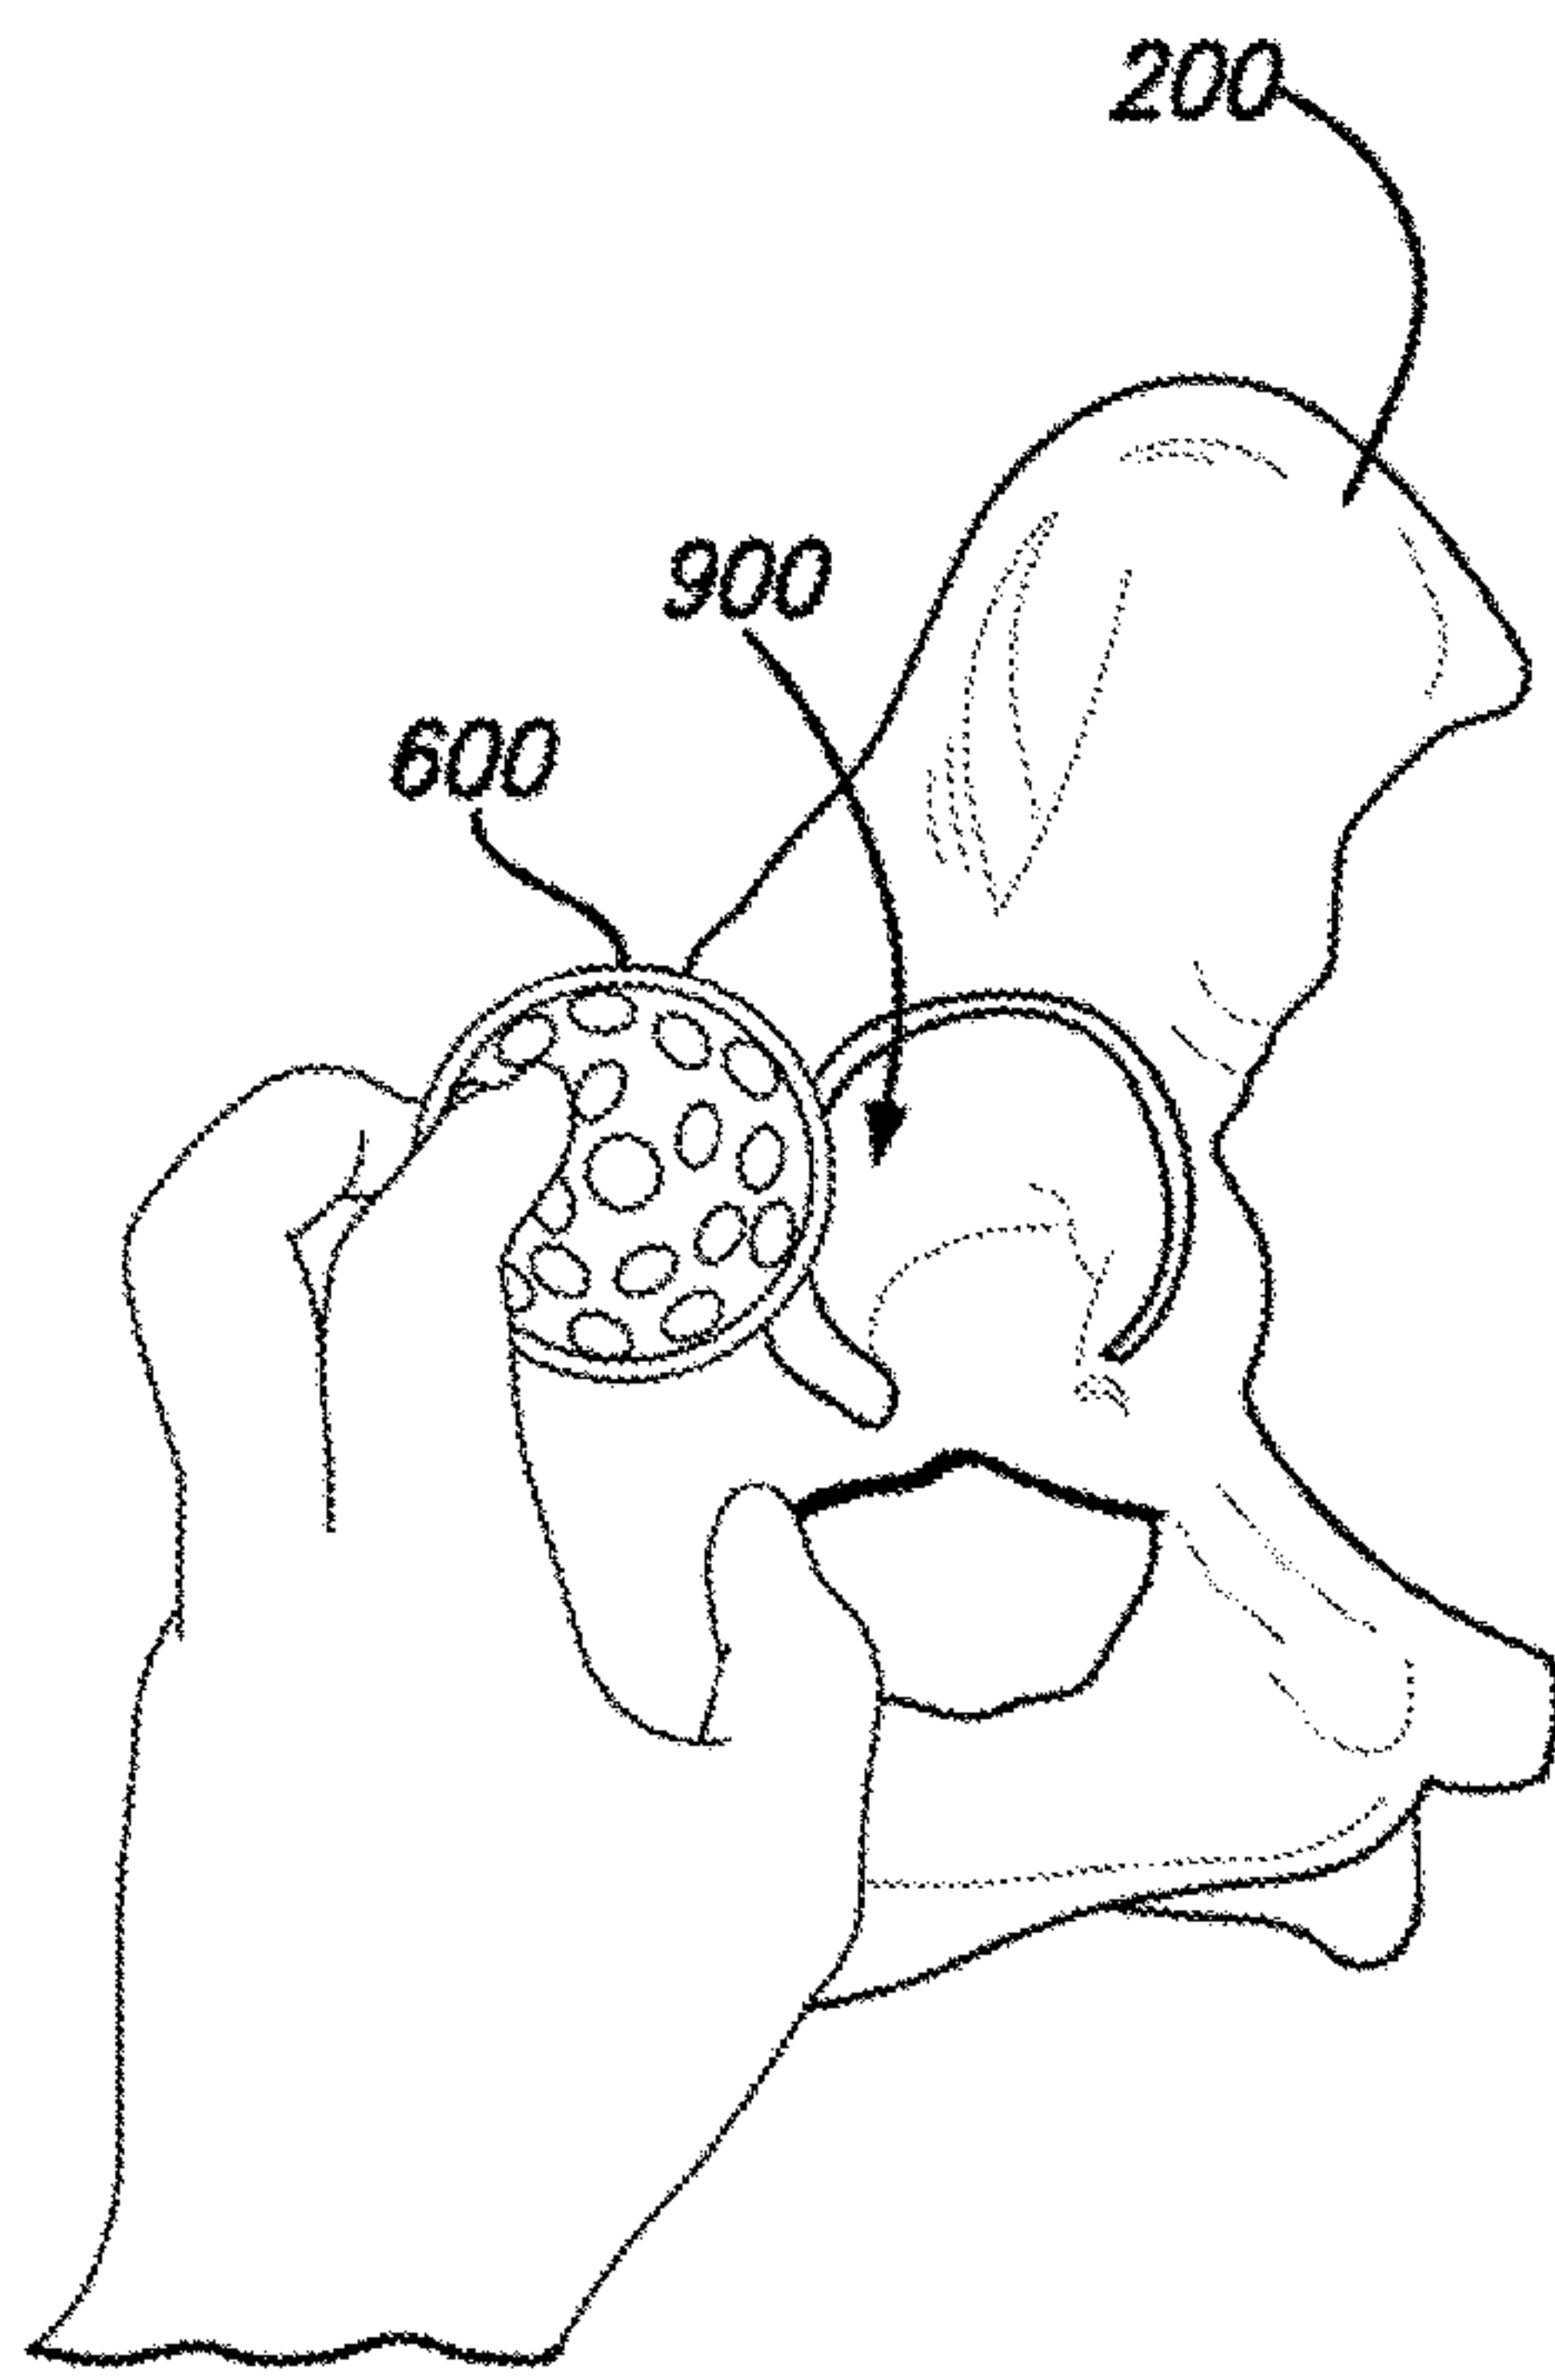


FIG. 12A

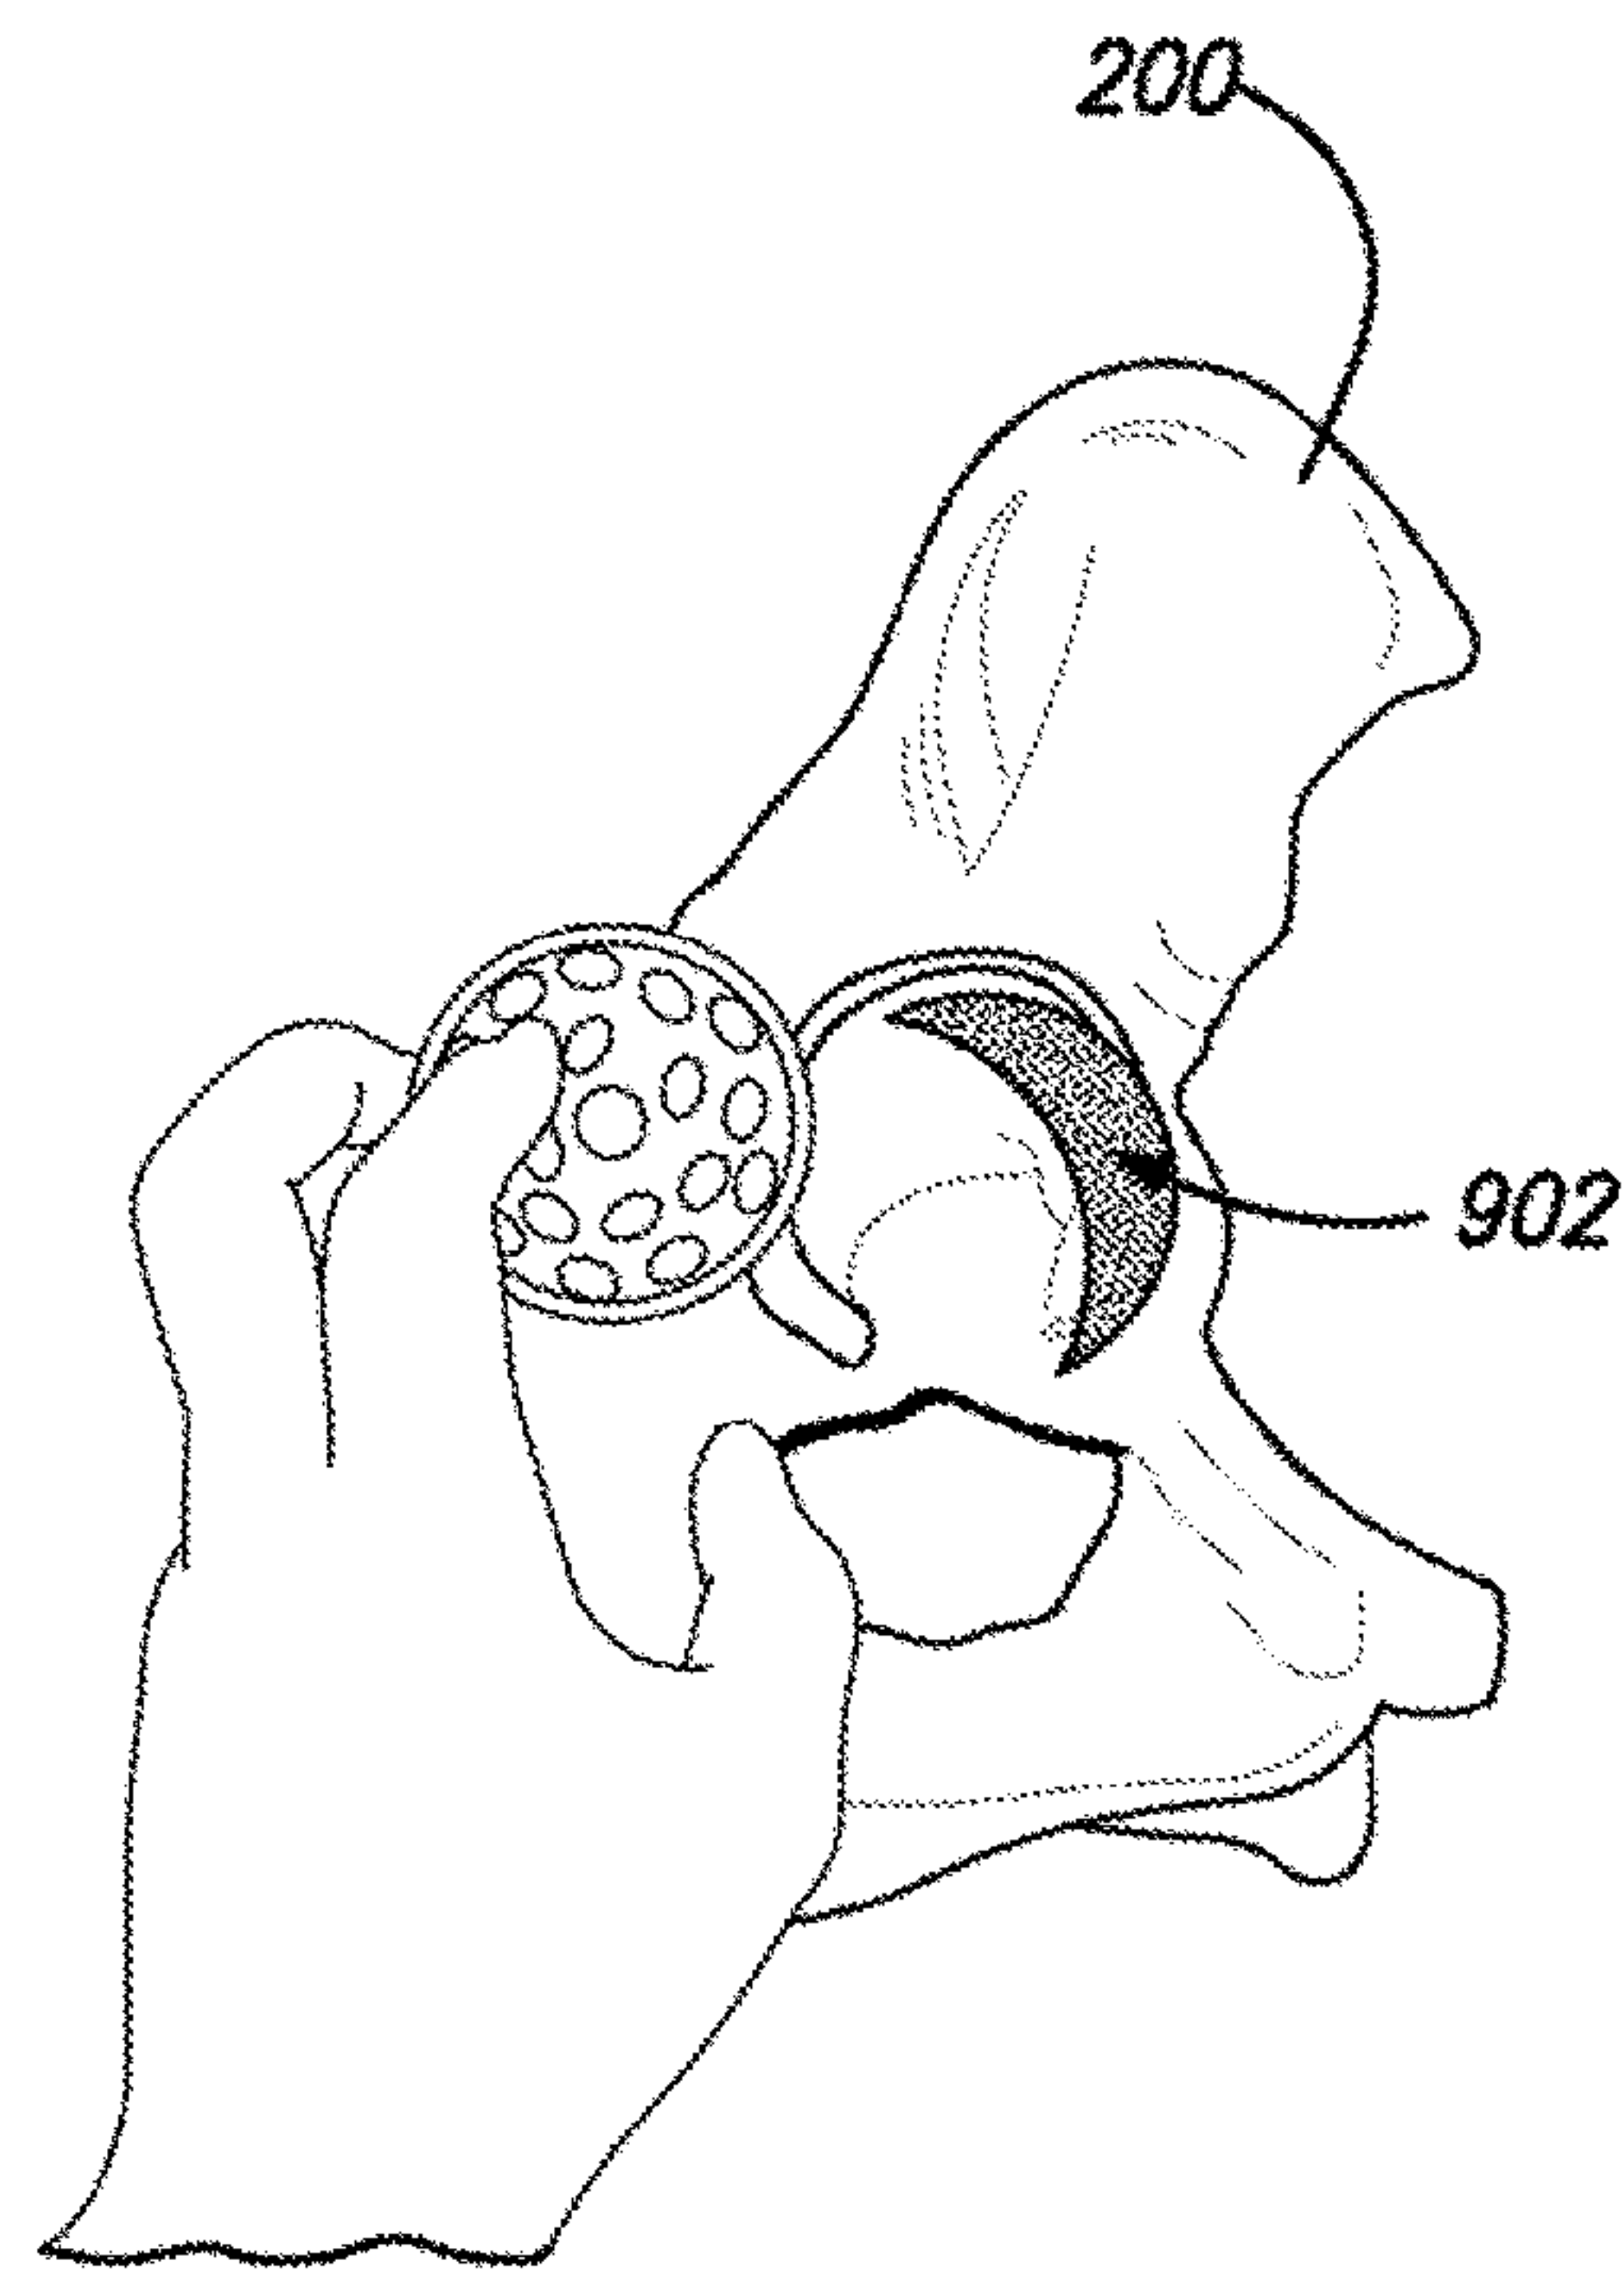


FIG. 12B

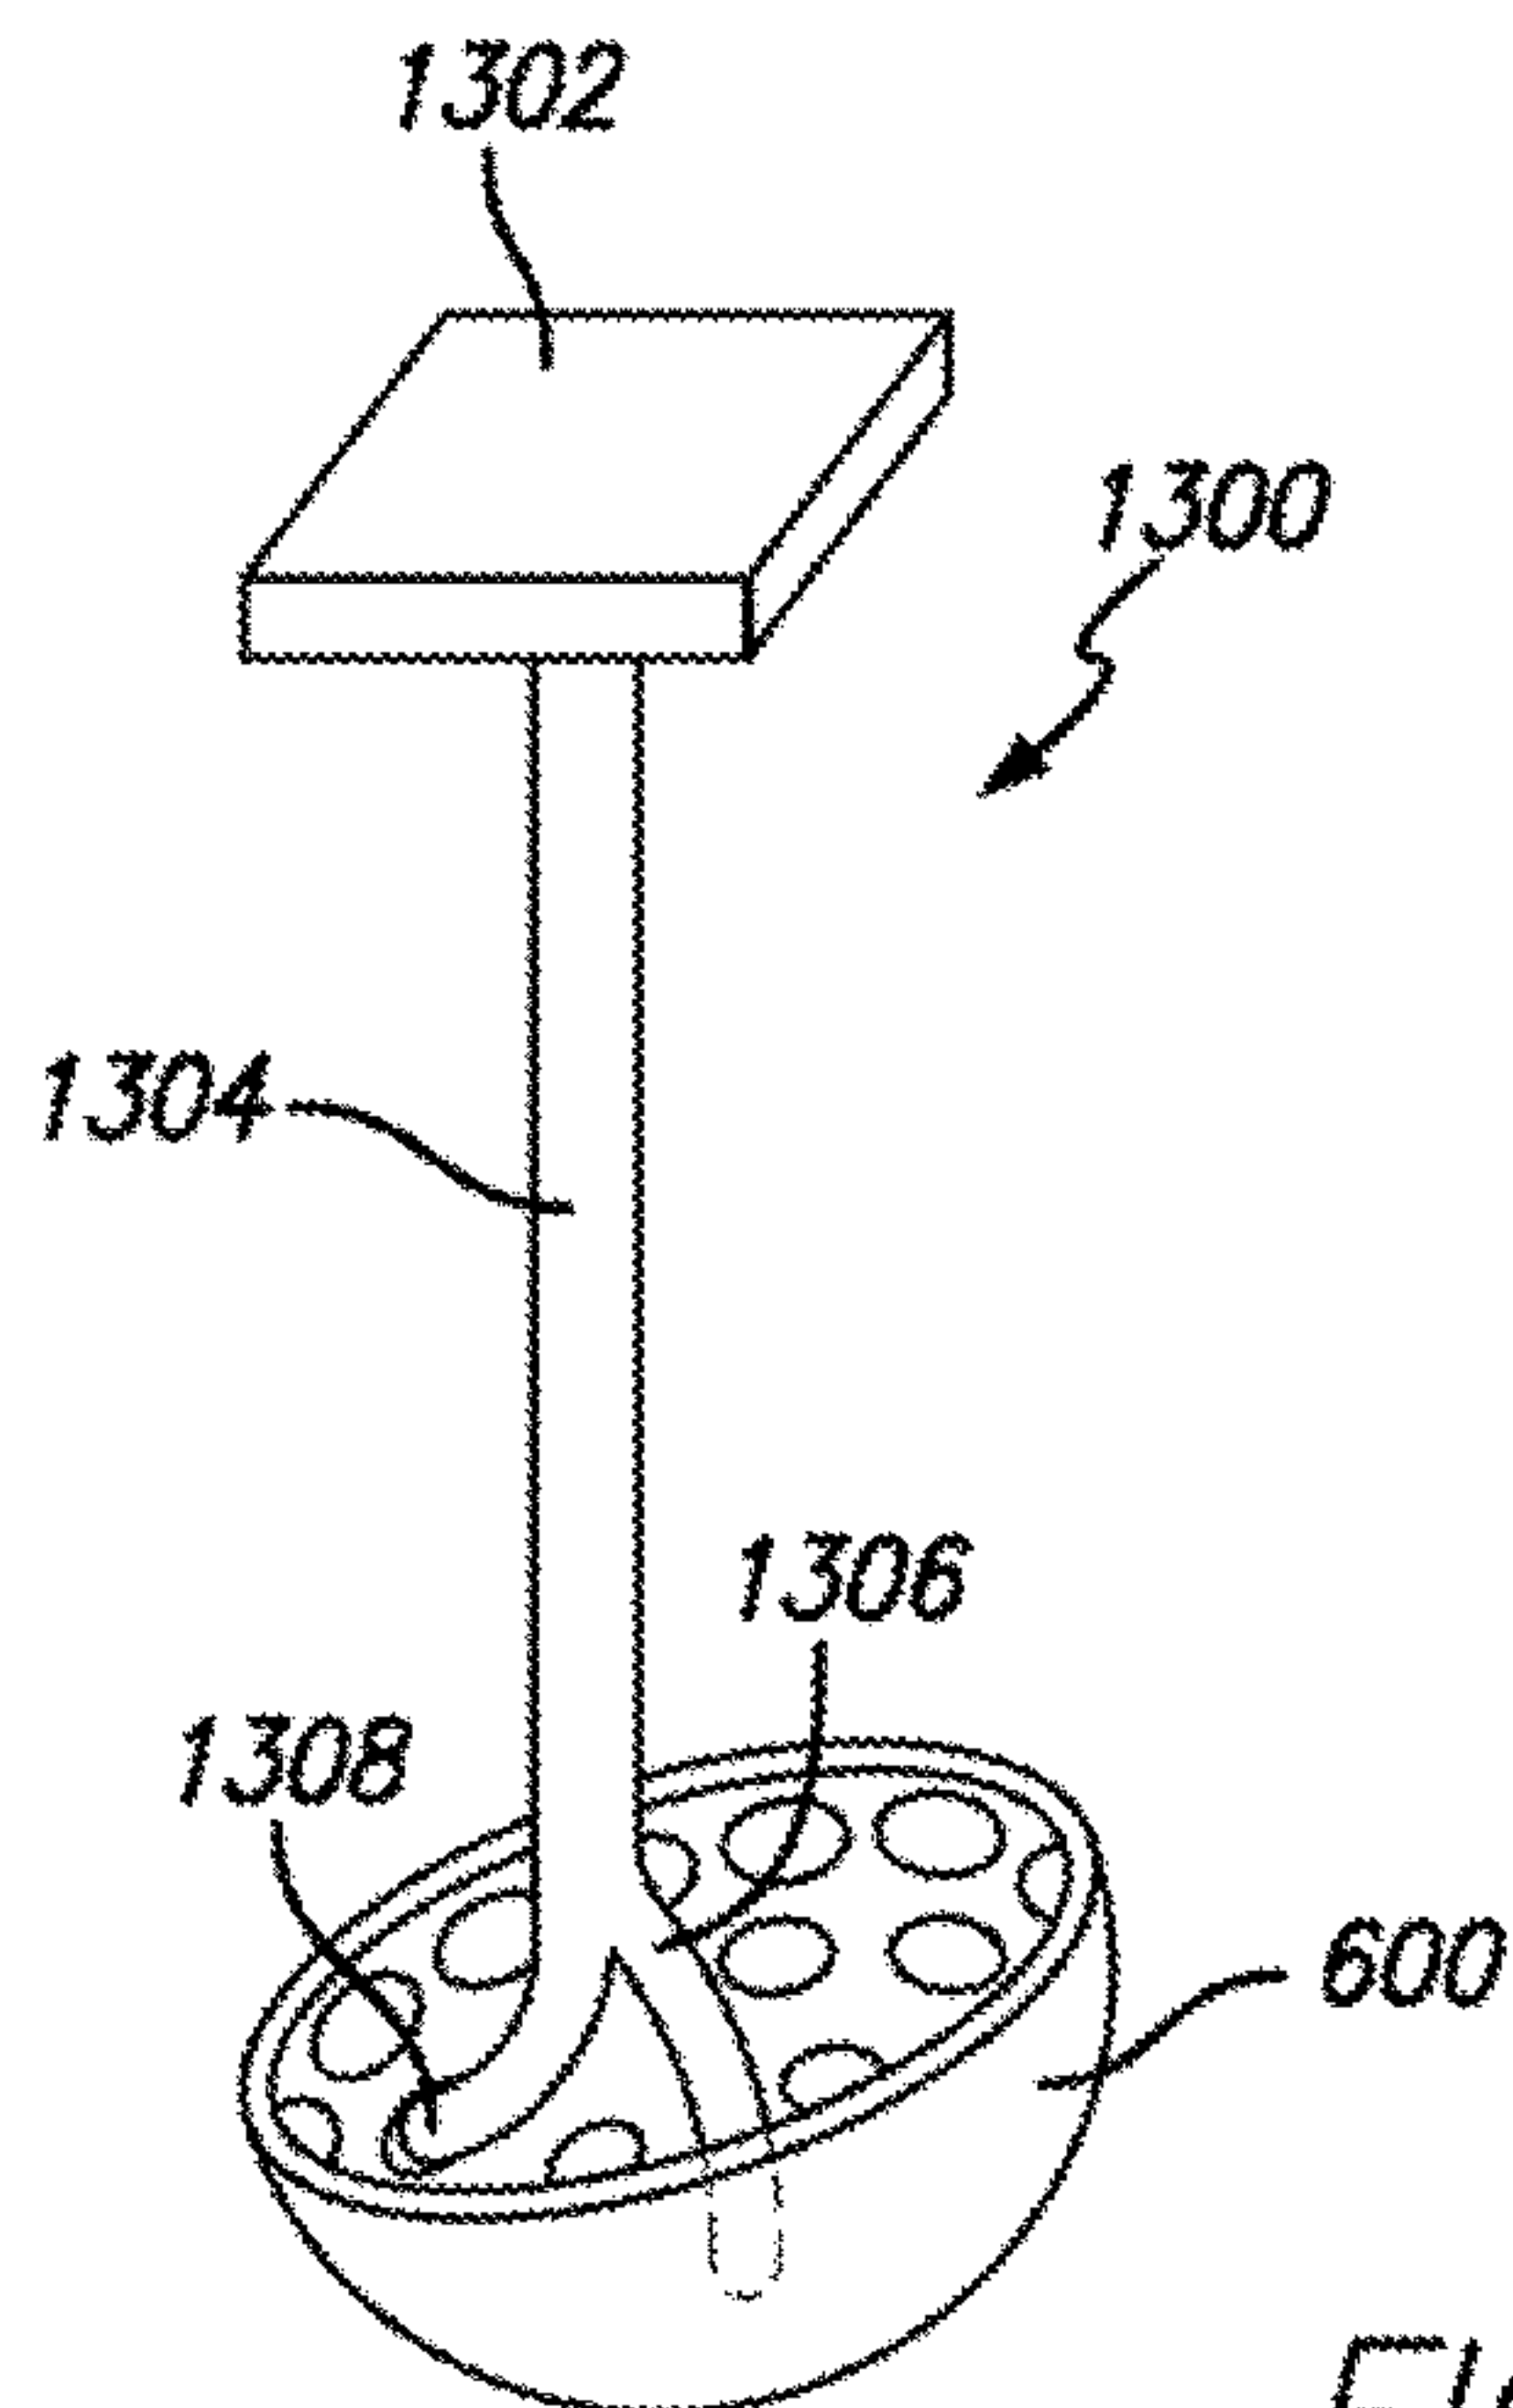


FIG. 13



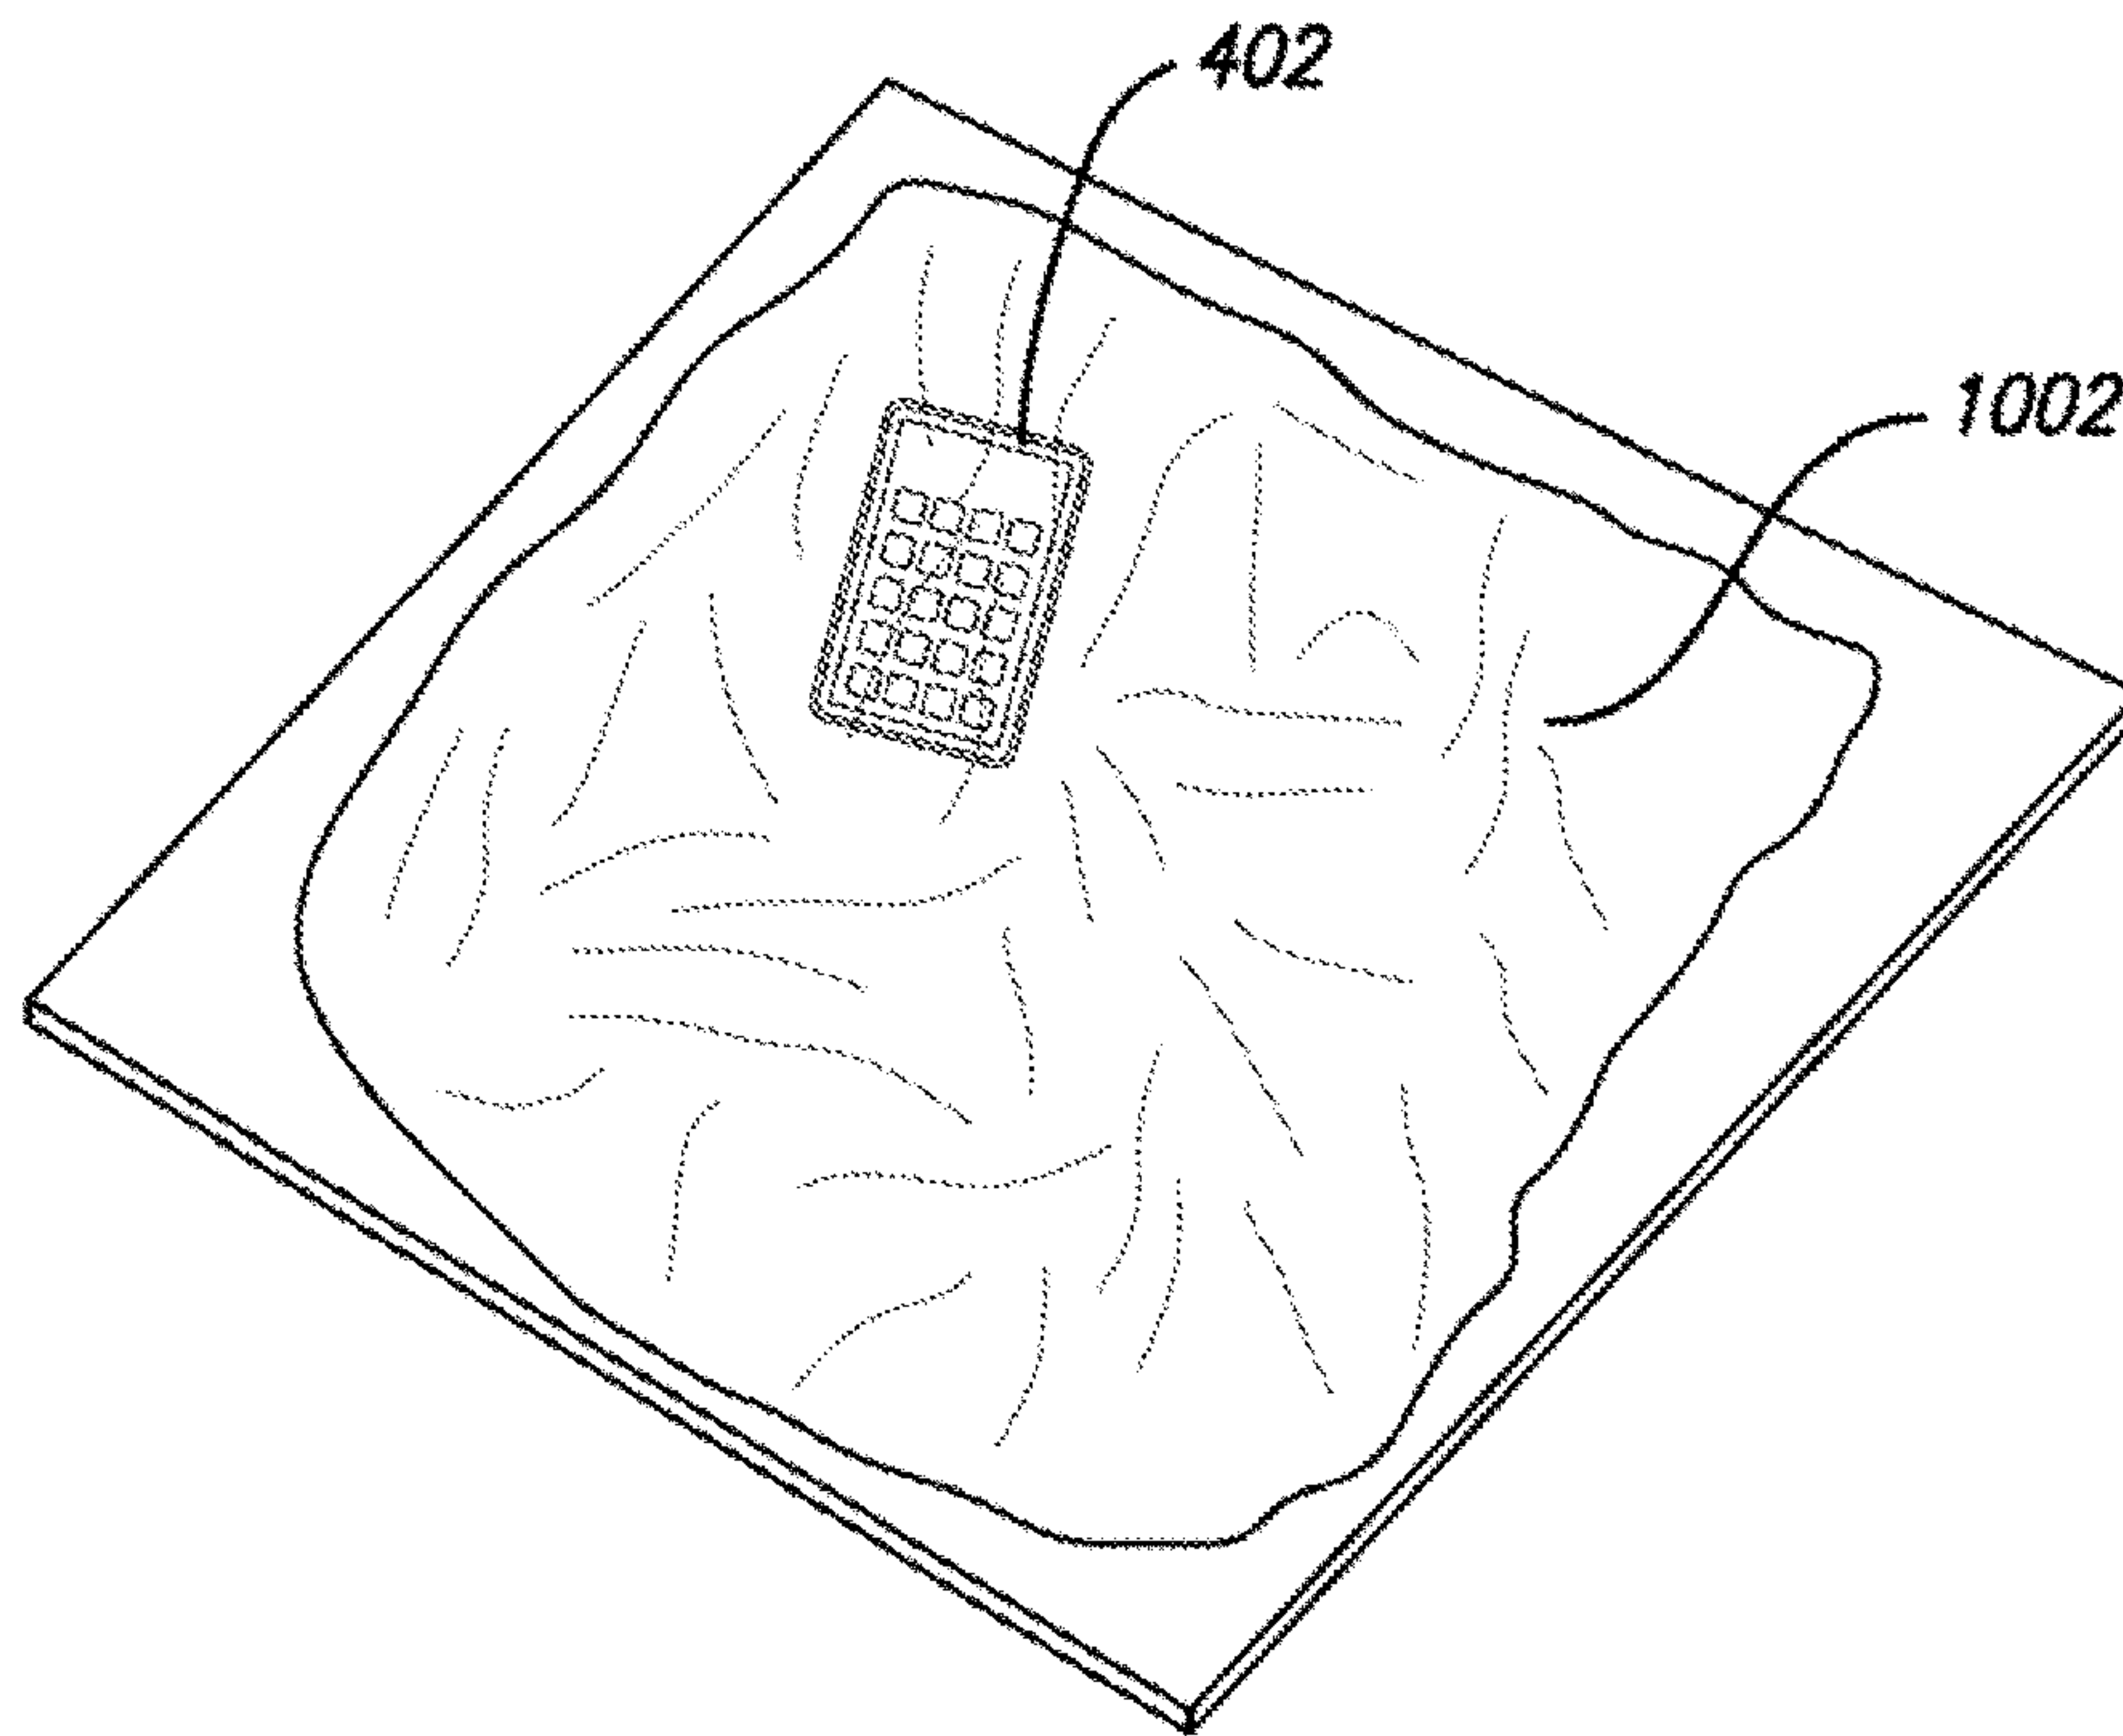


FIG. 14A

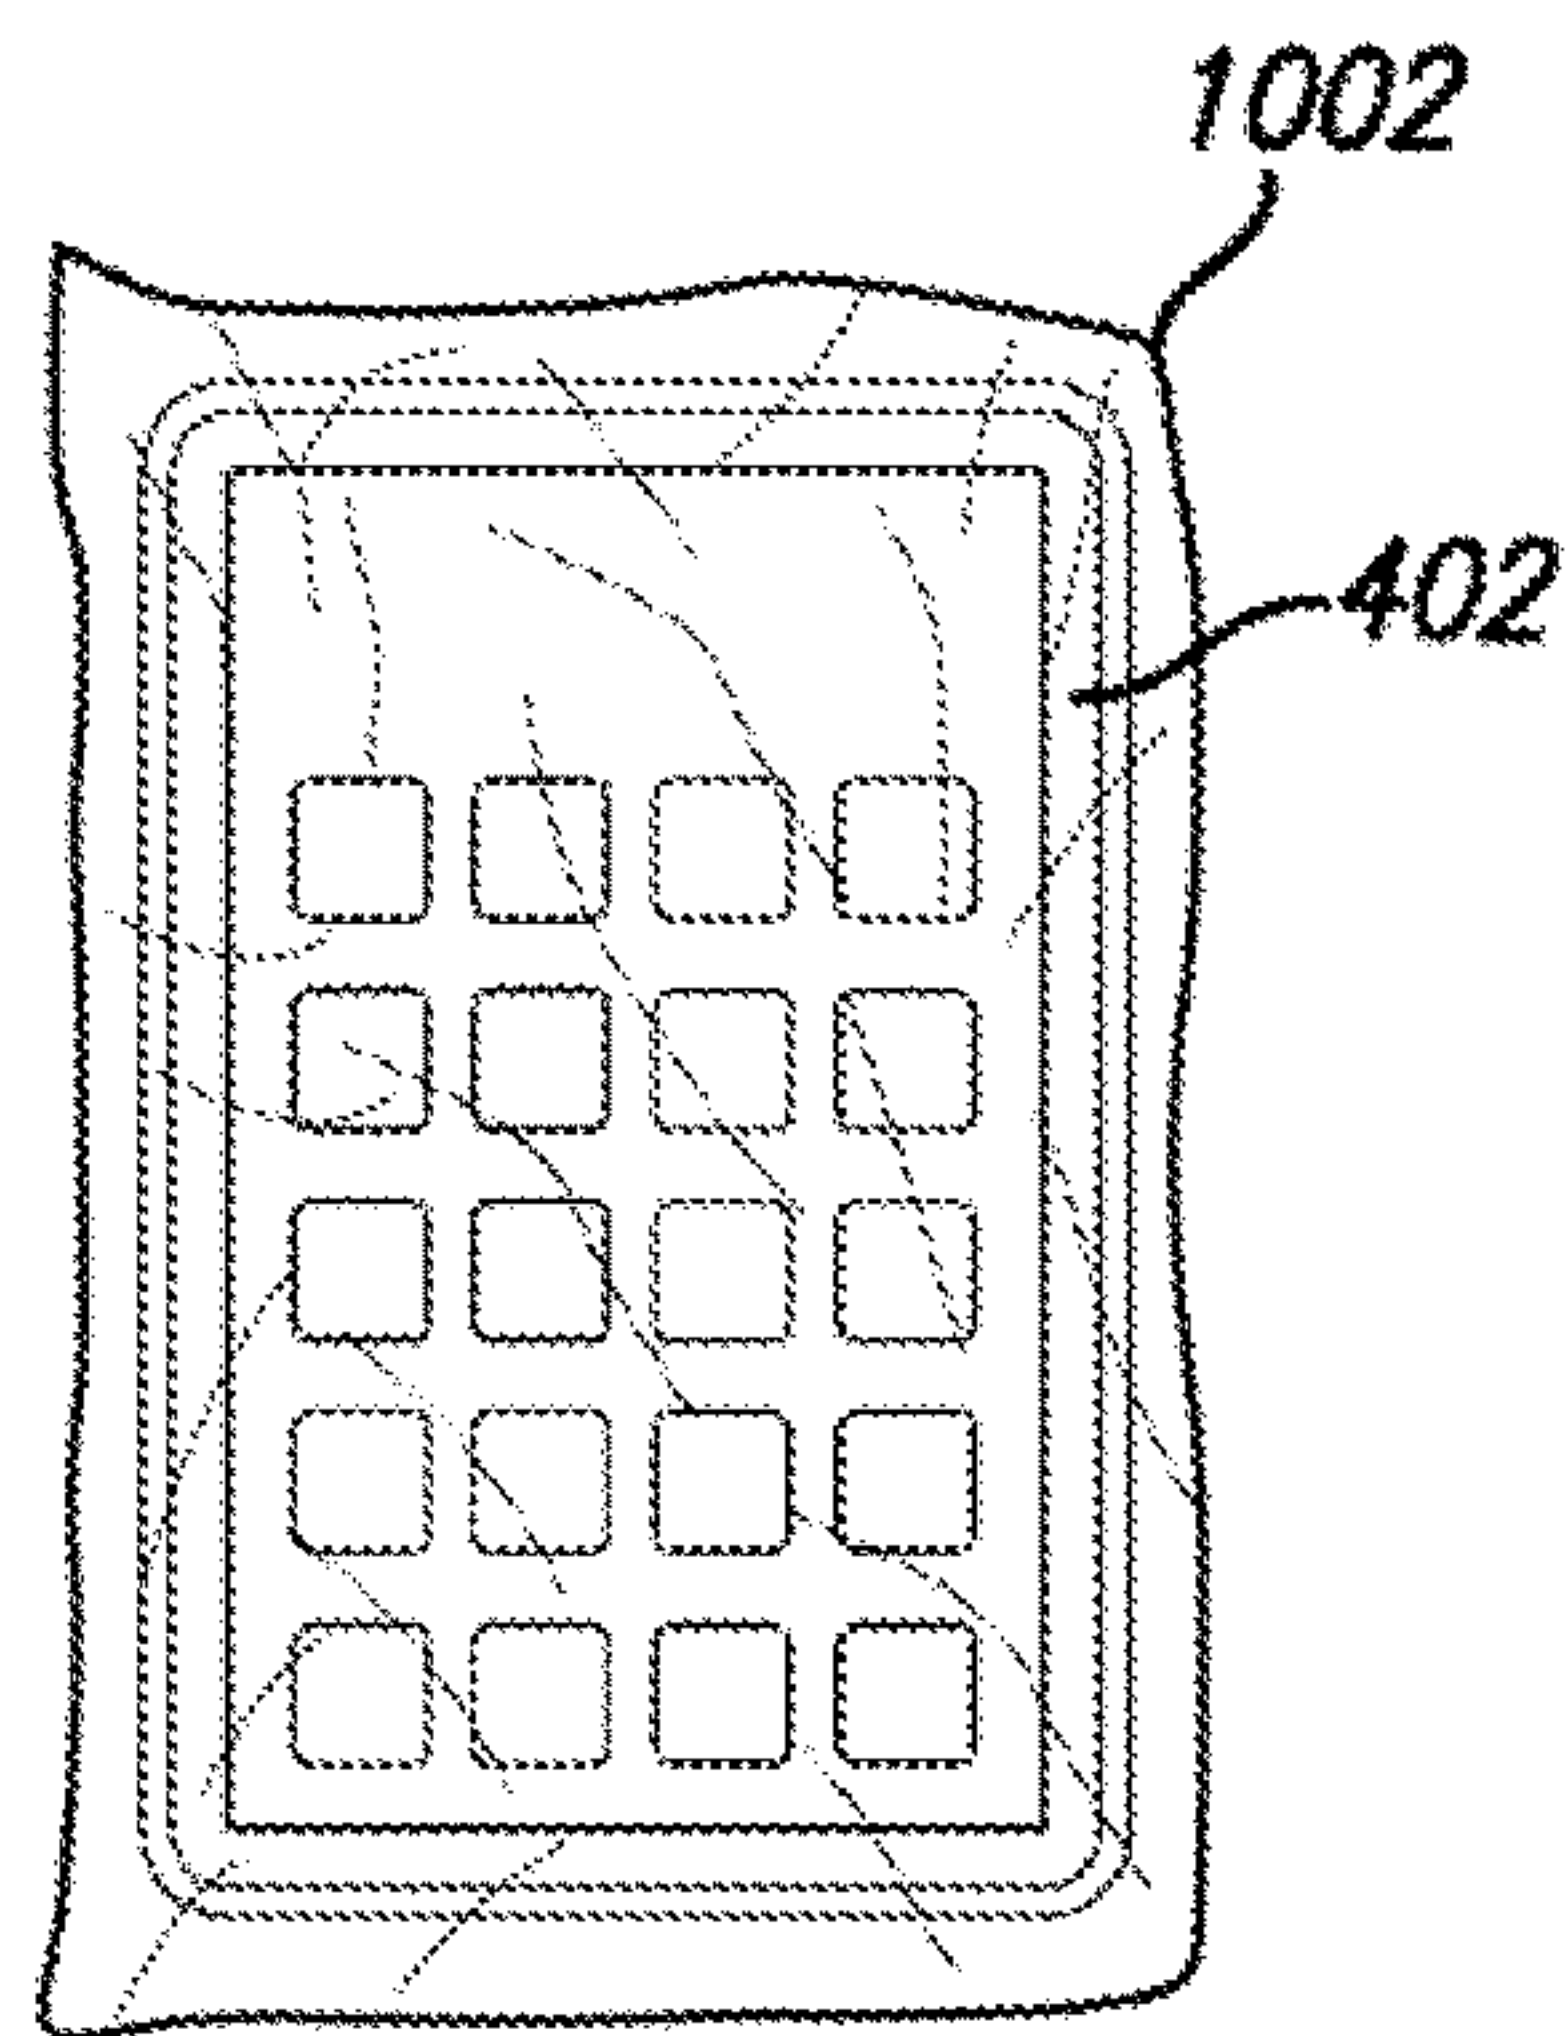
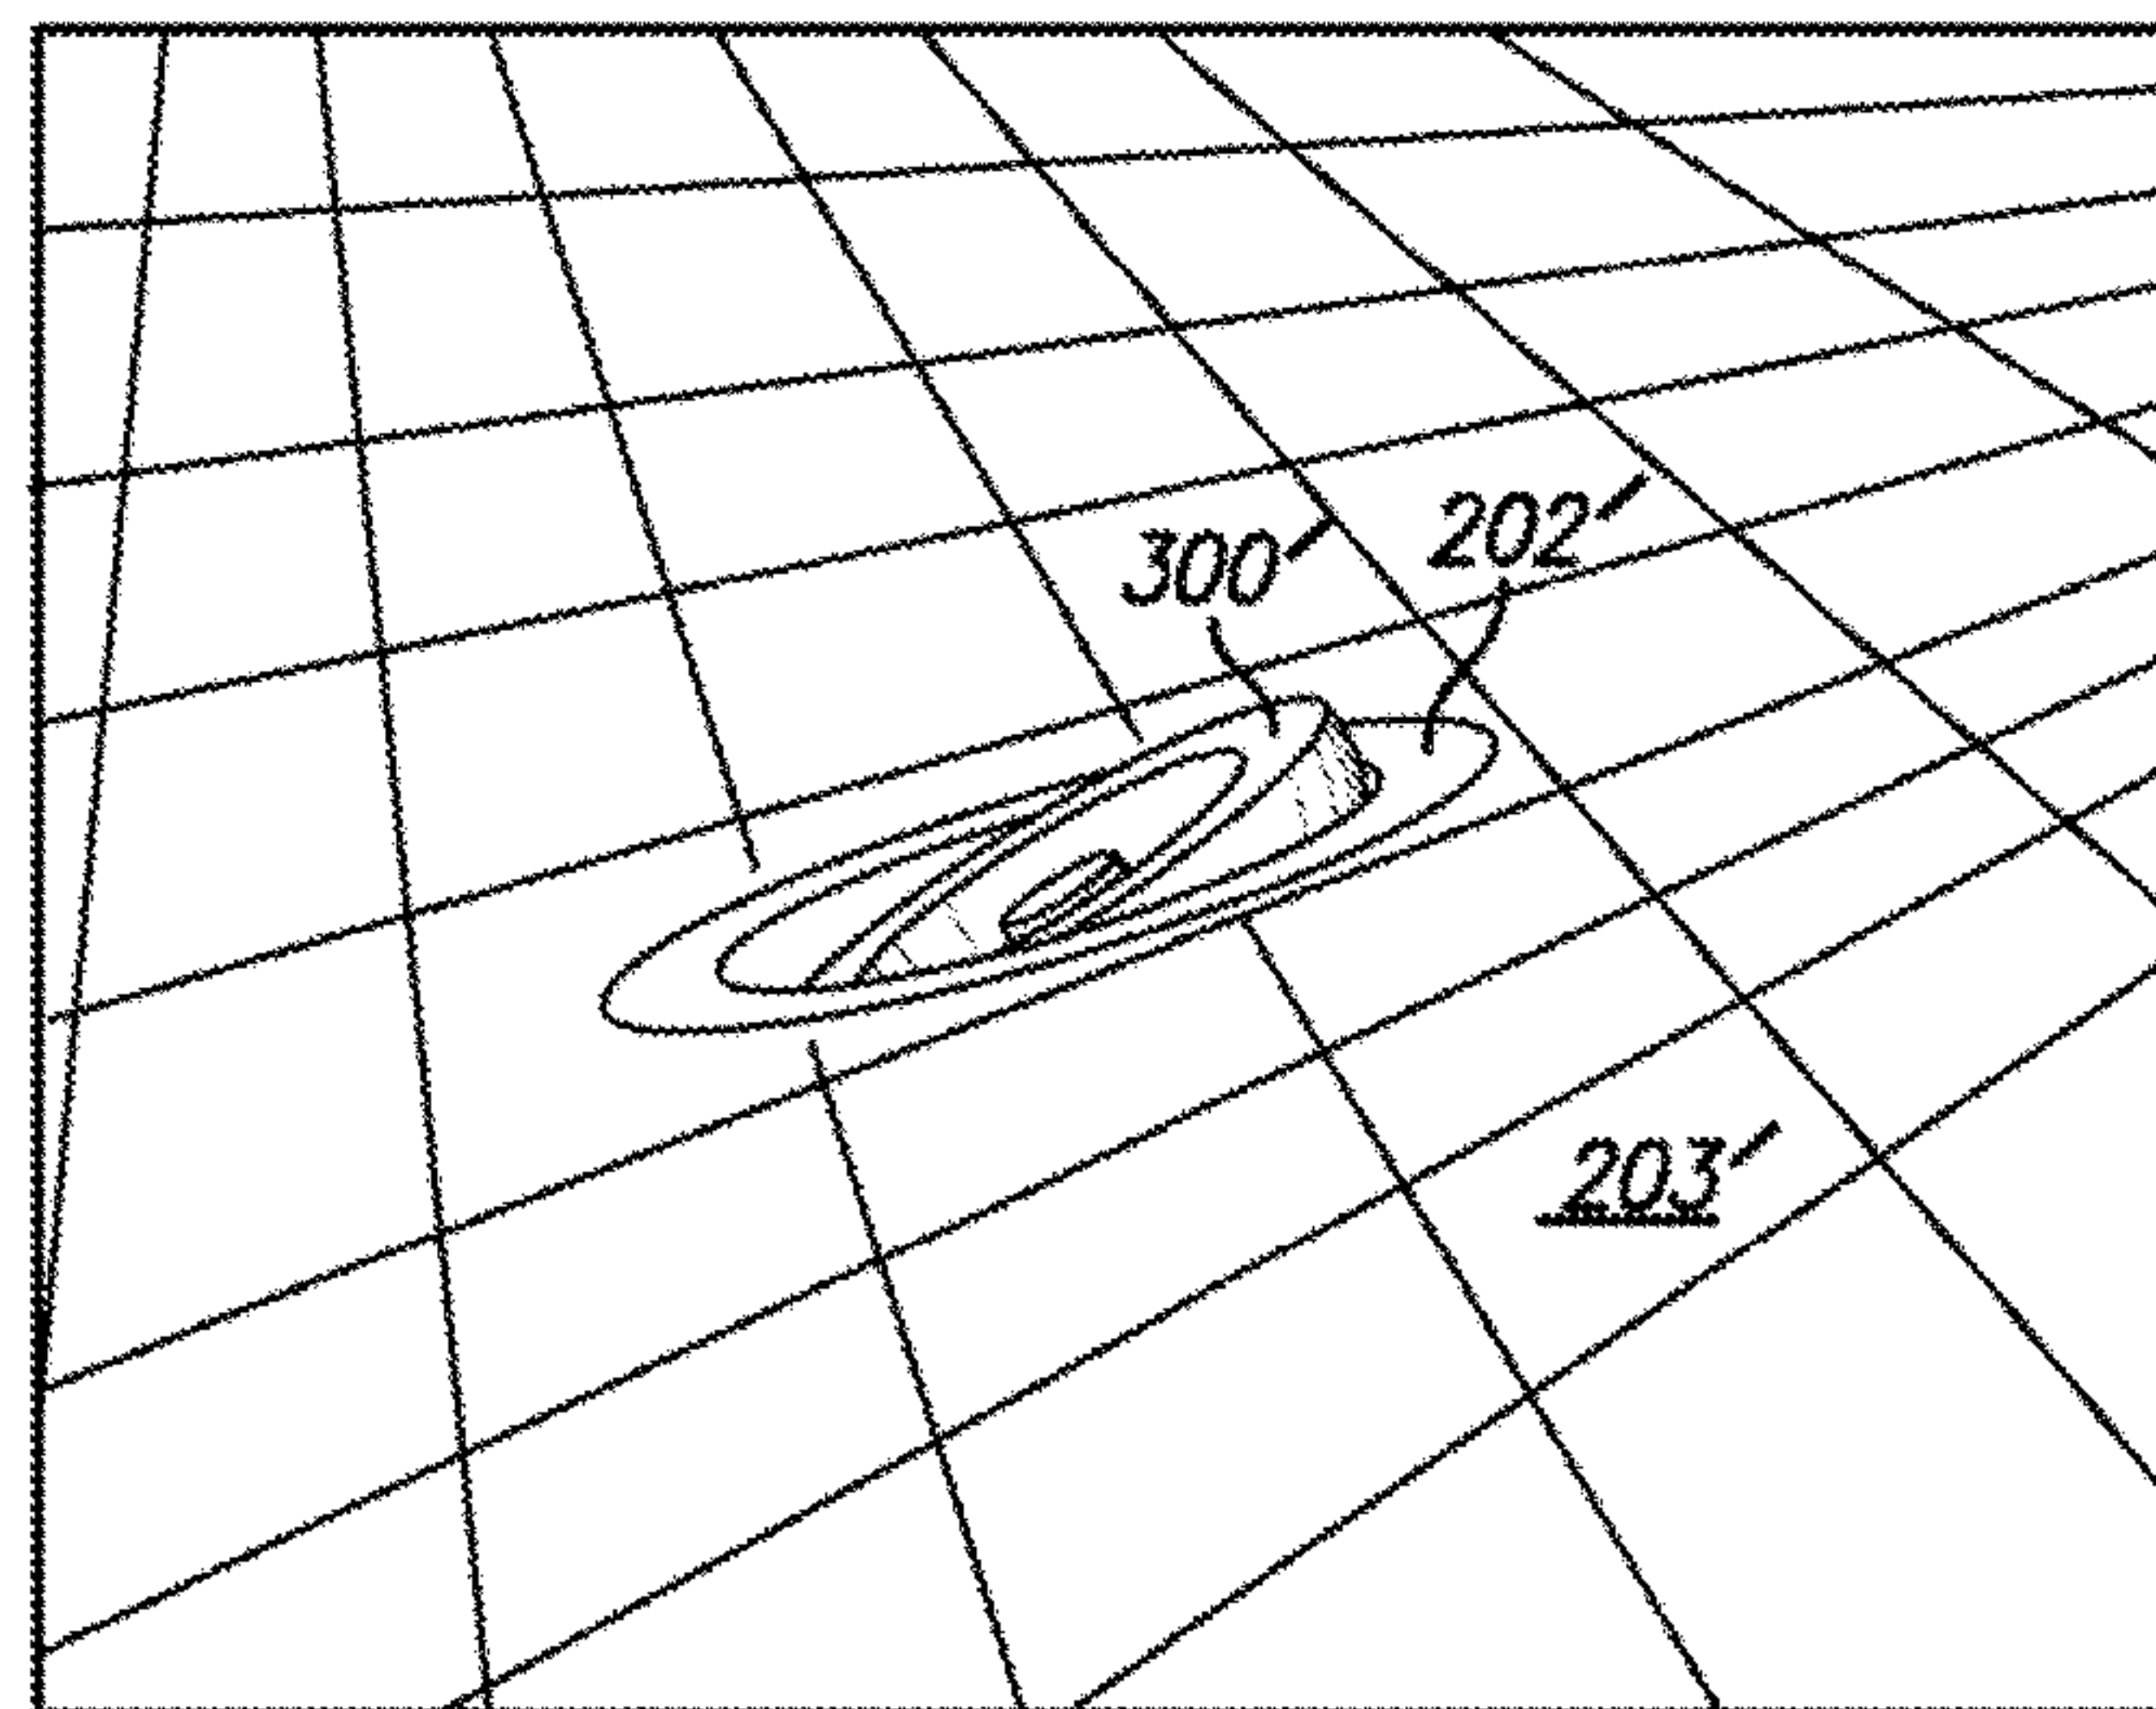
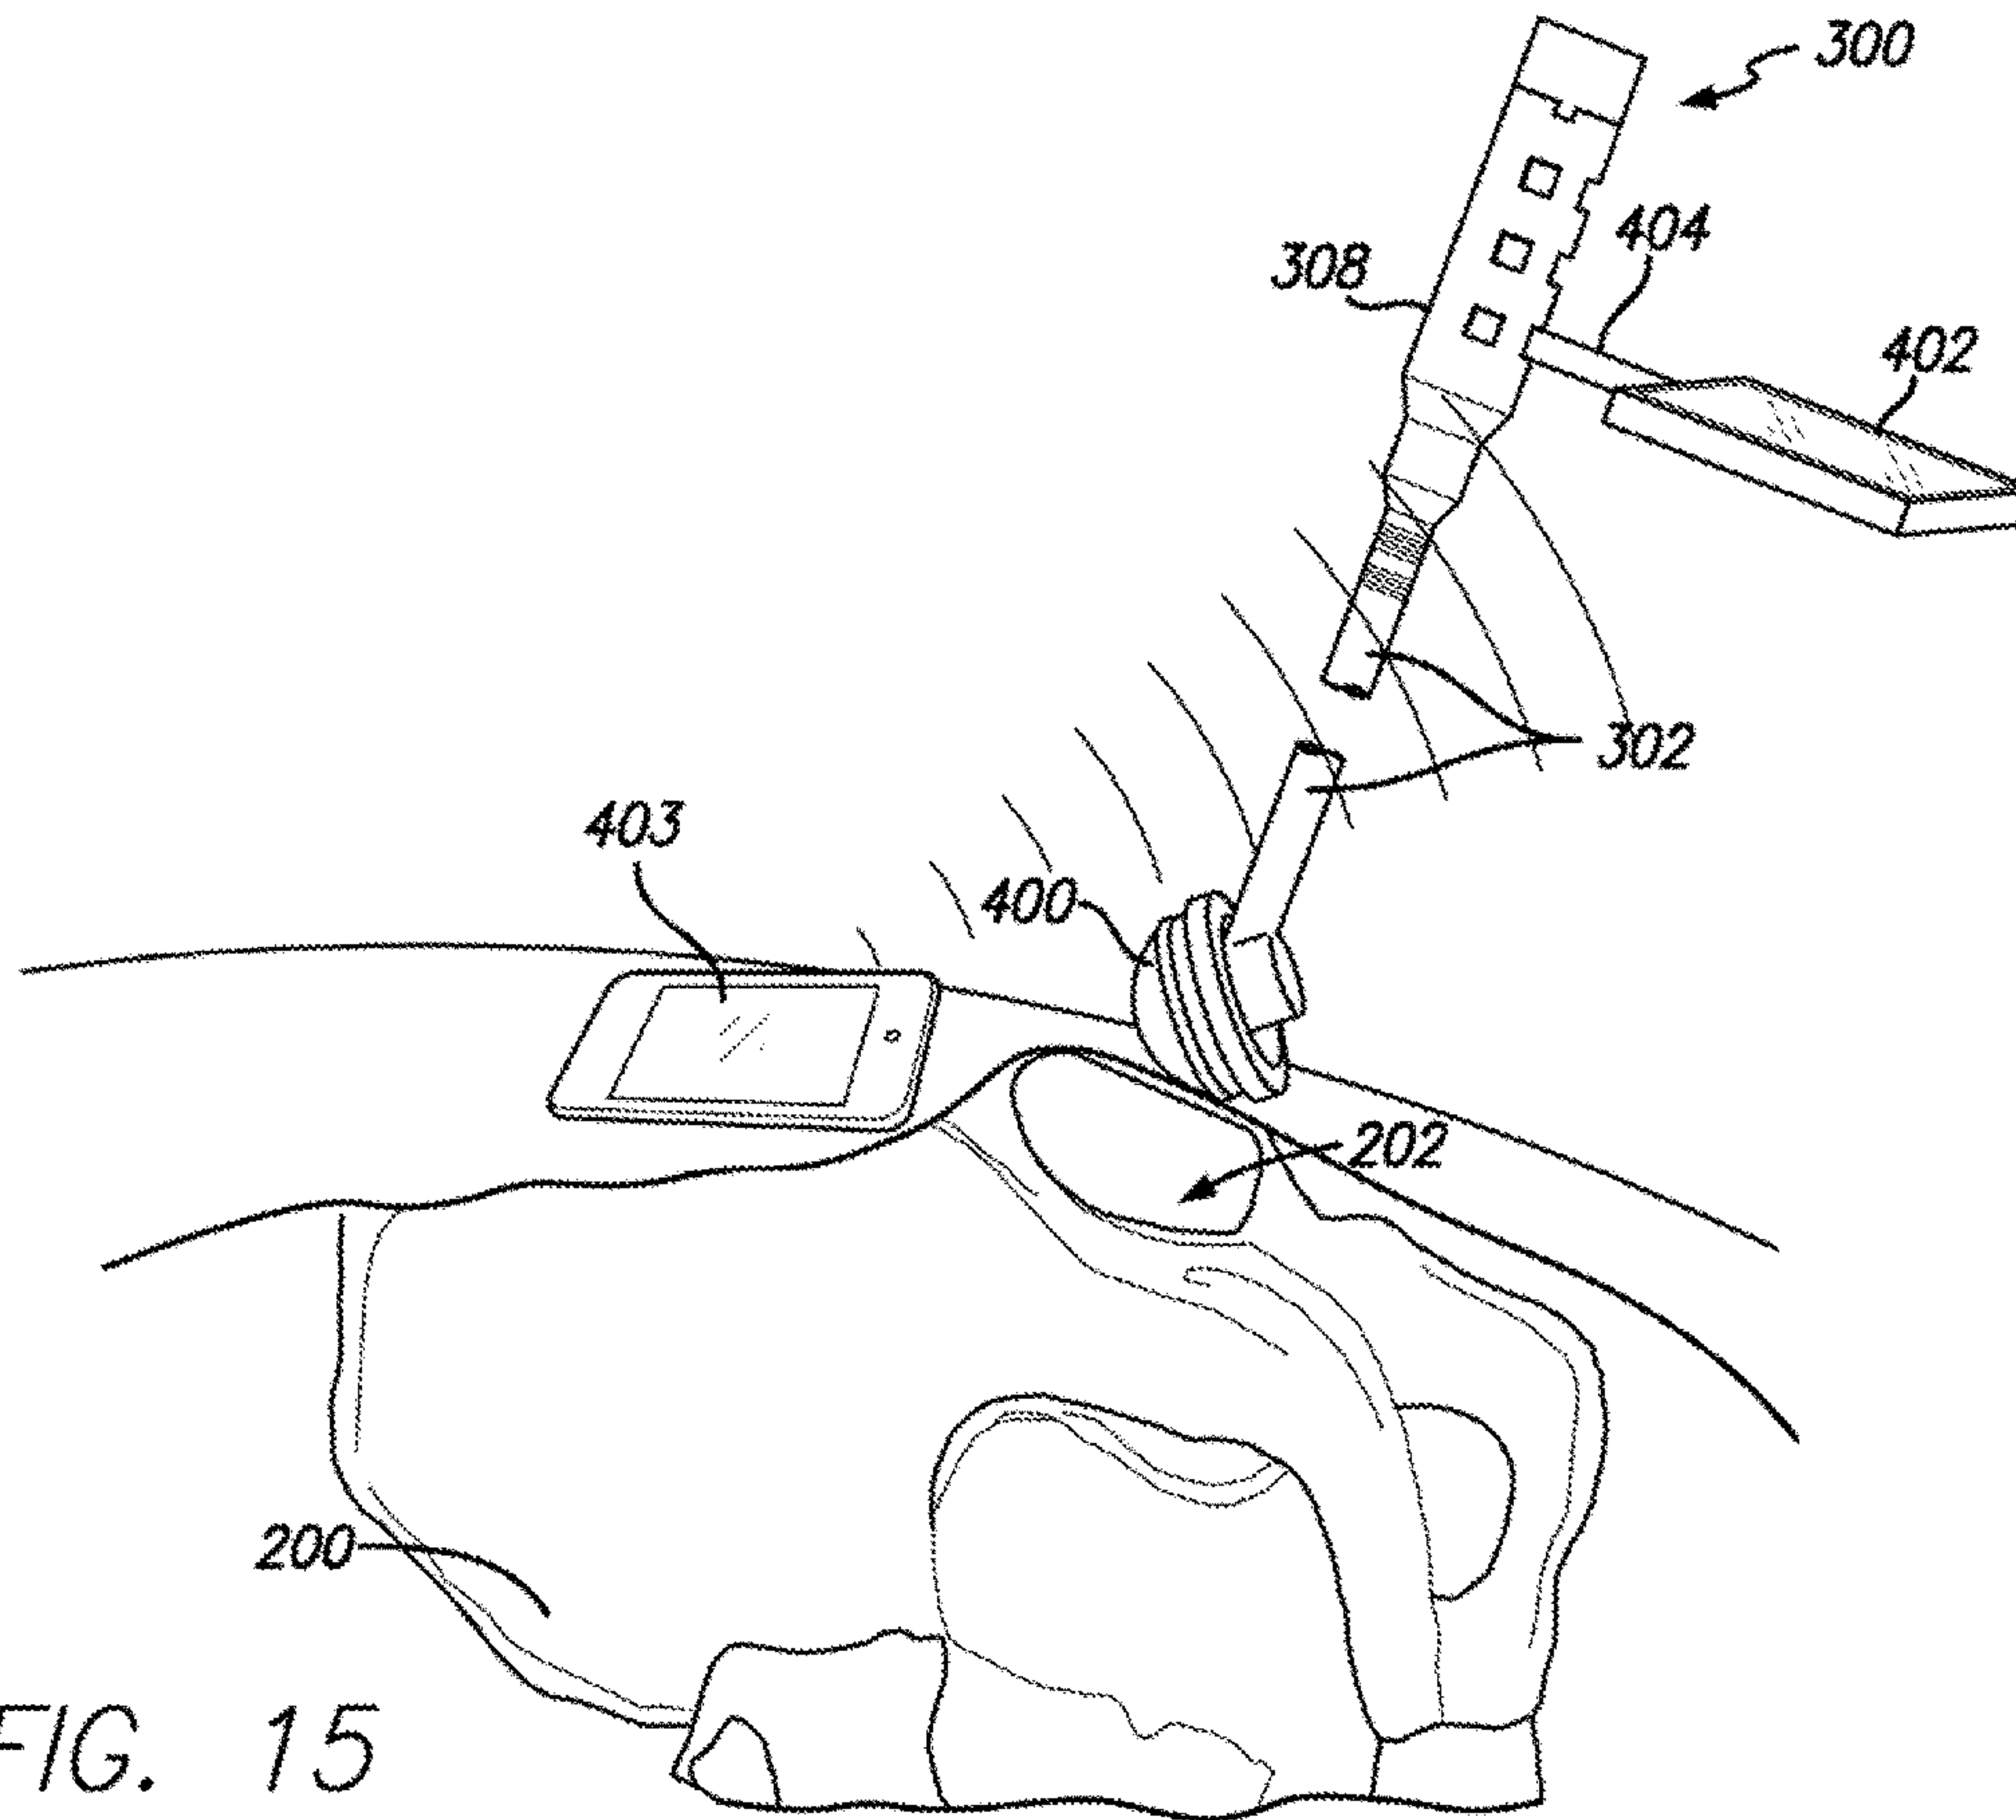


FIG. 14B



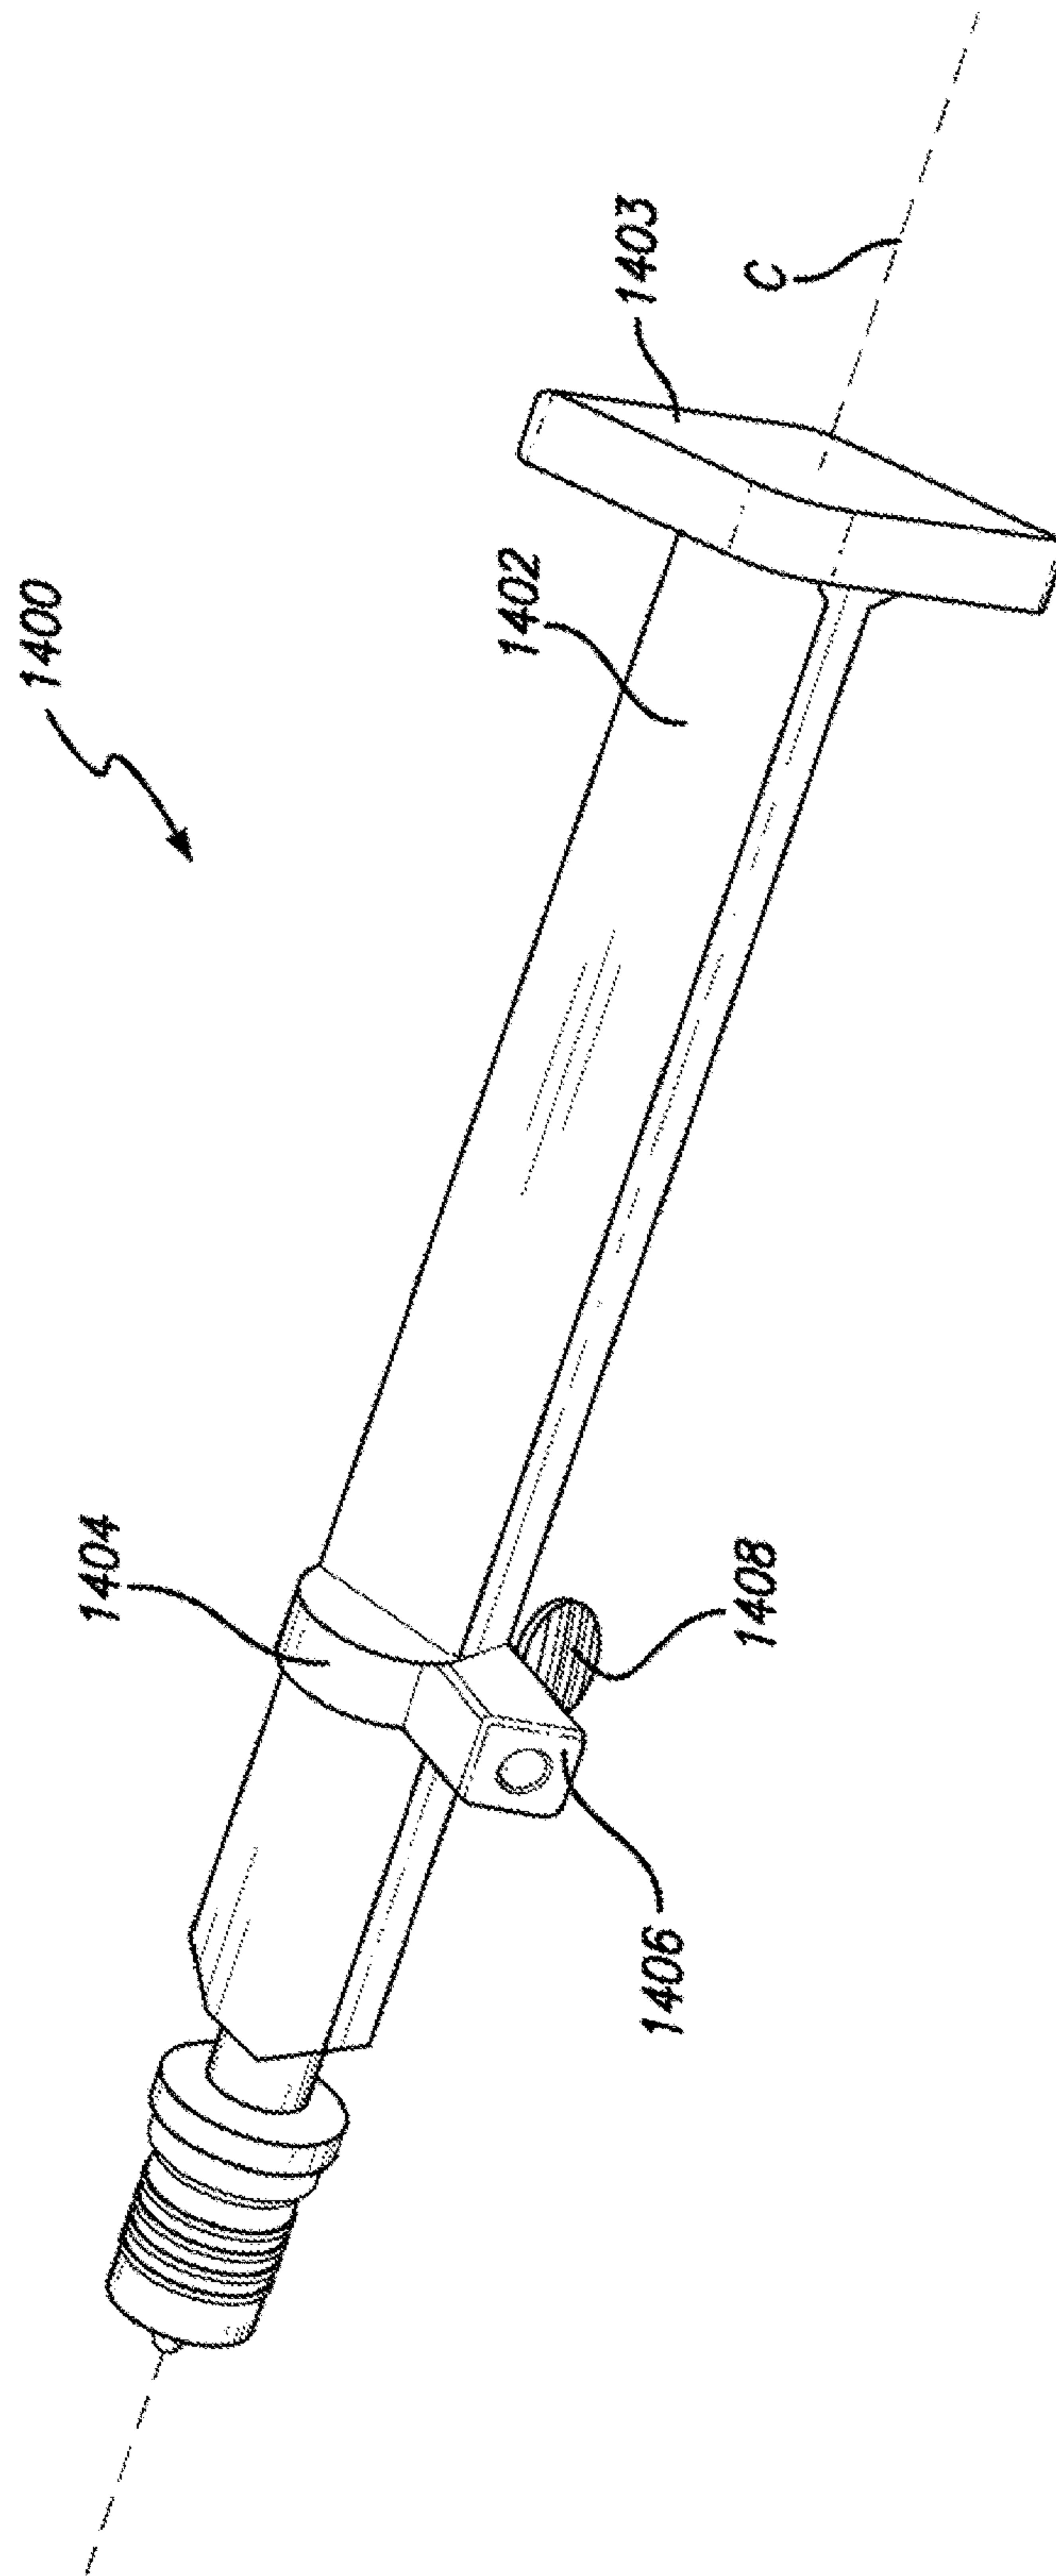


FIG. 17



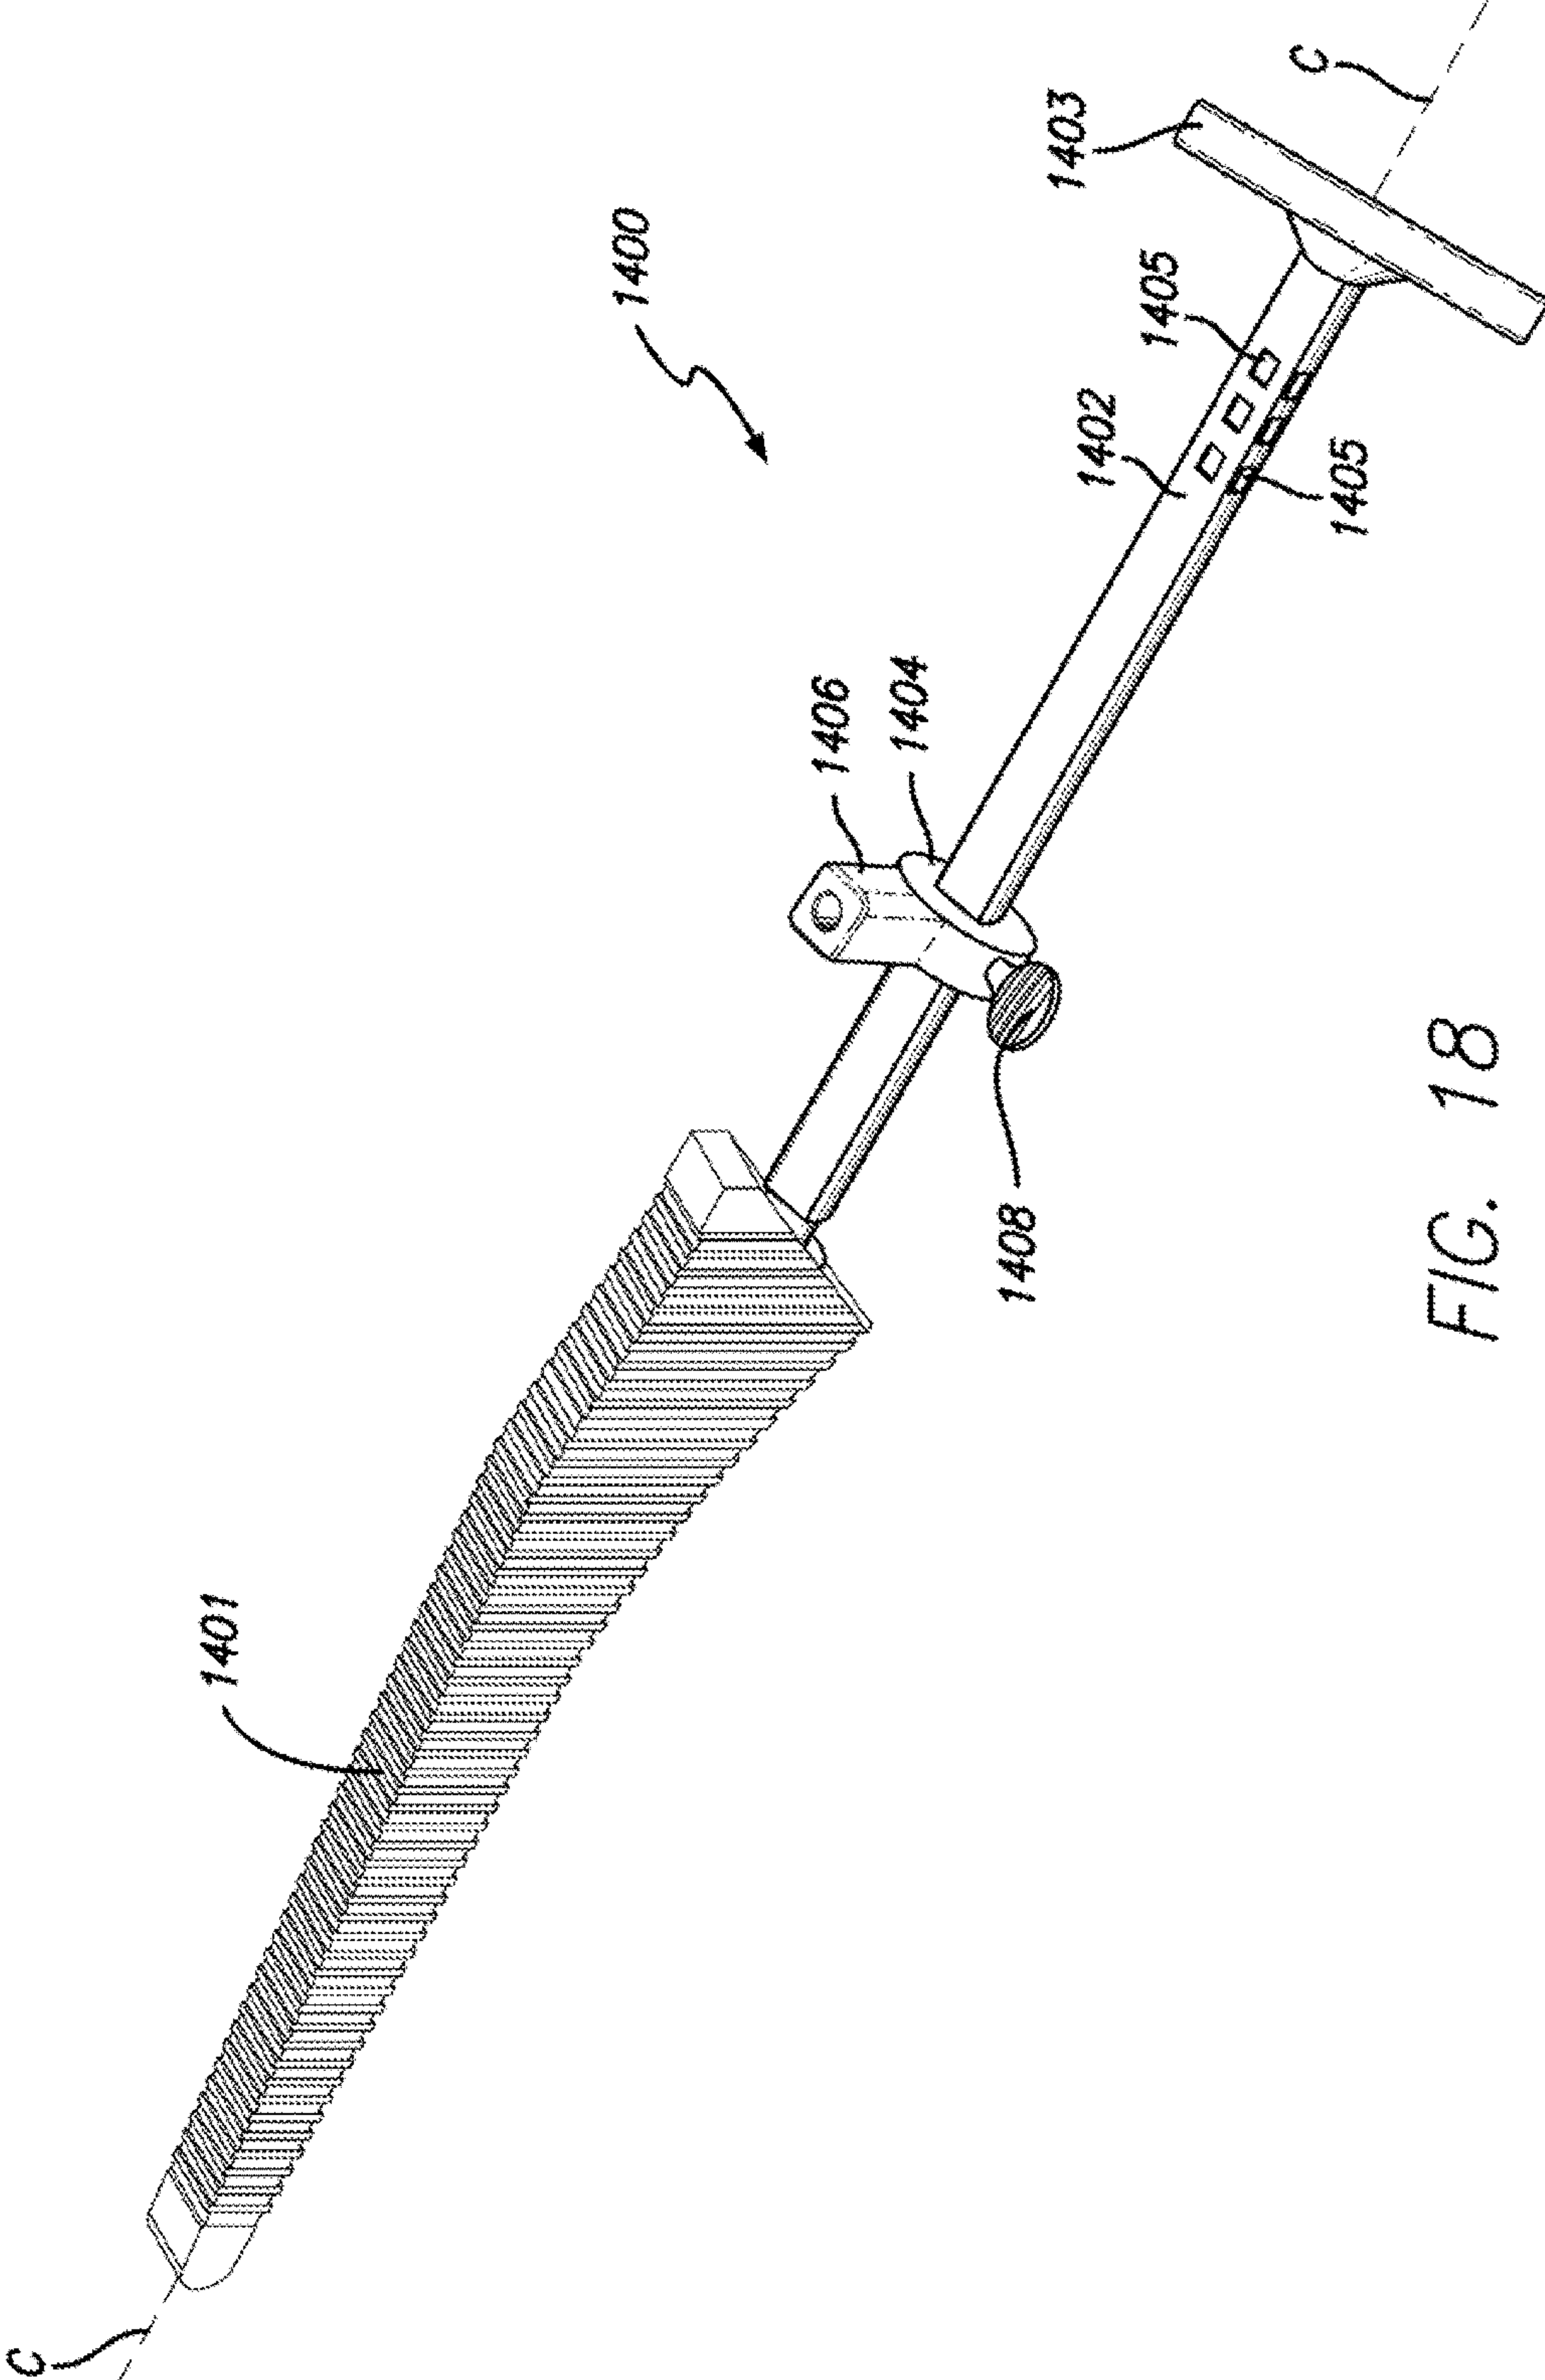


FIG. 18

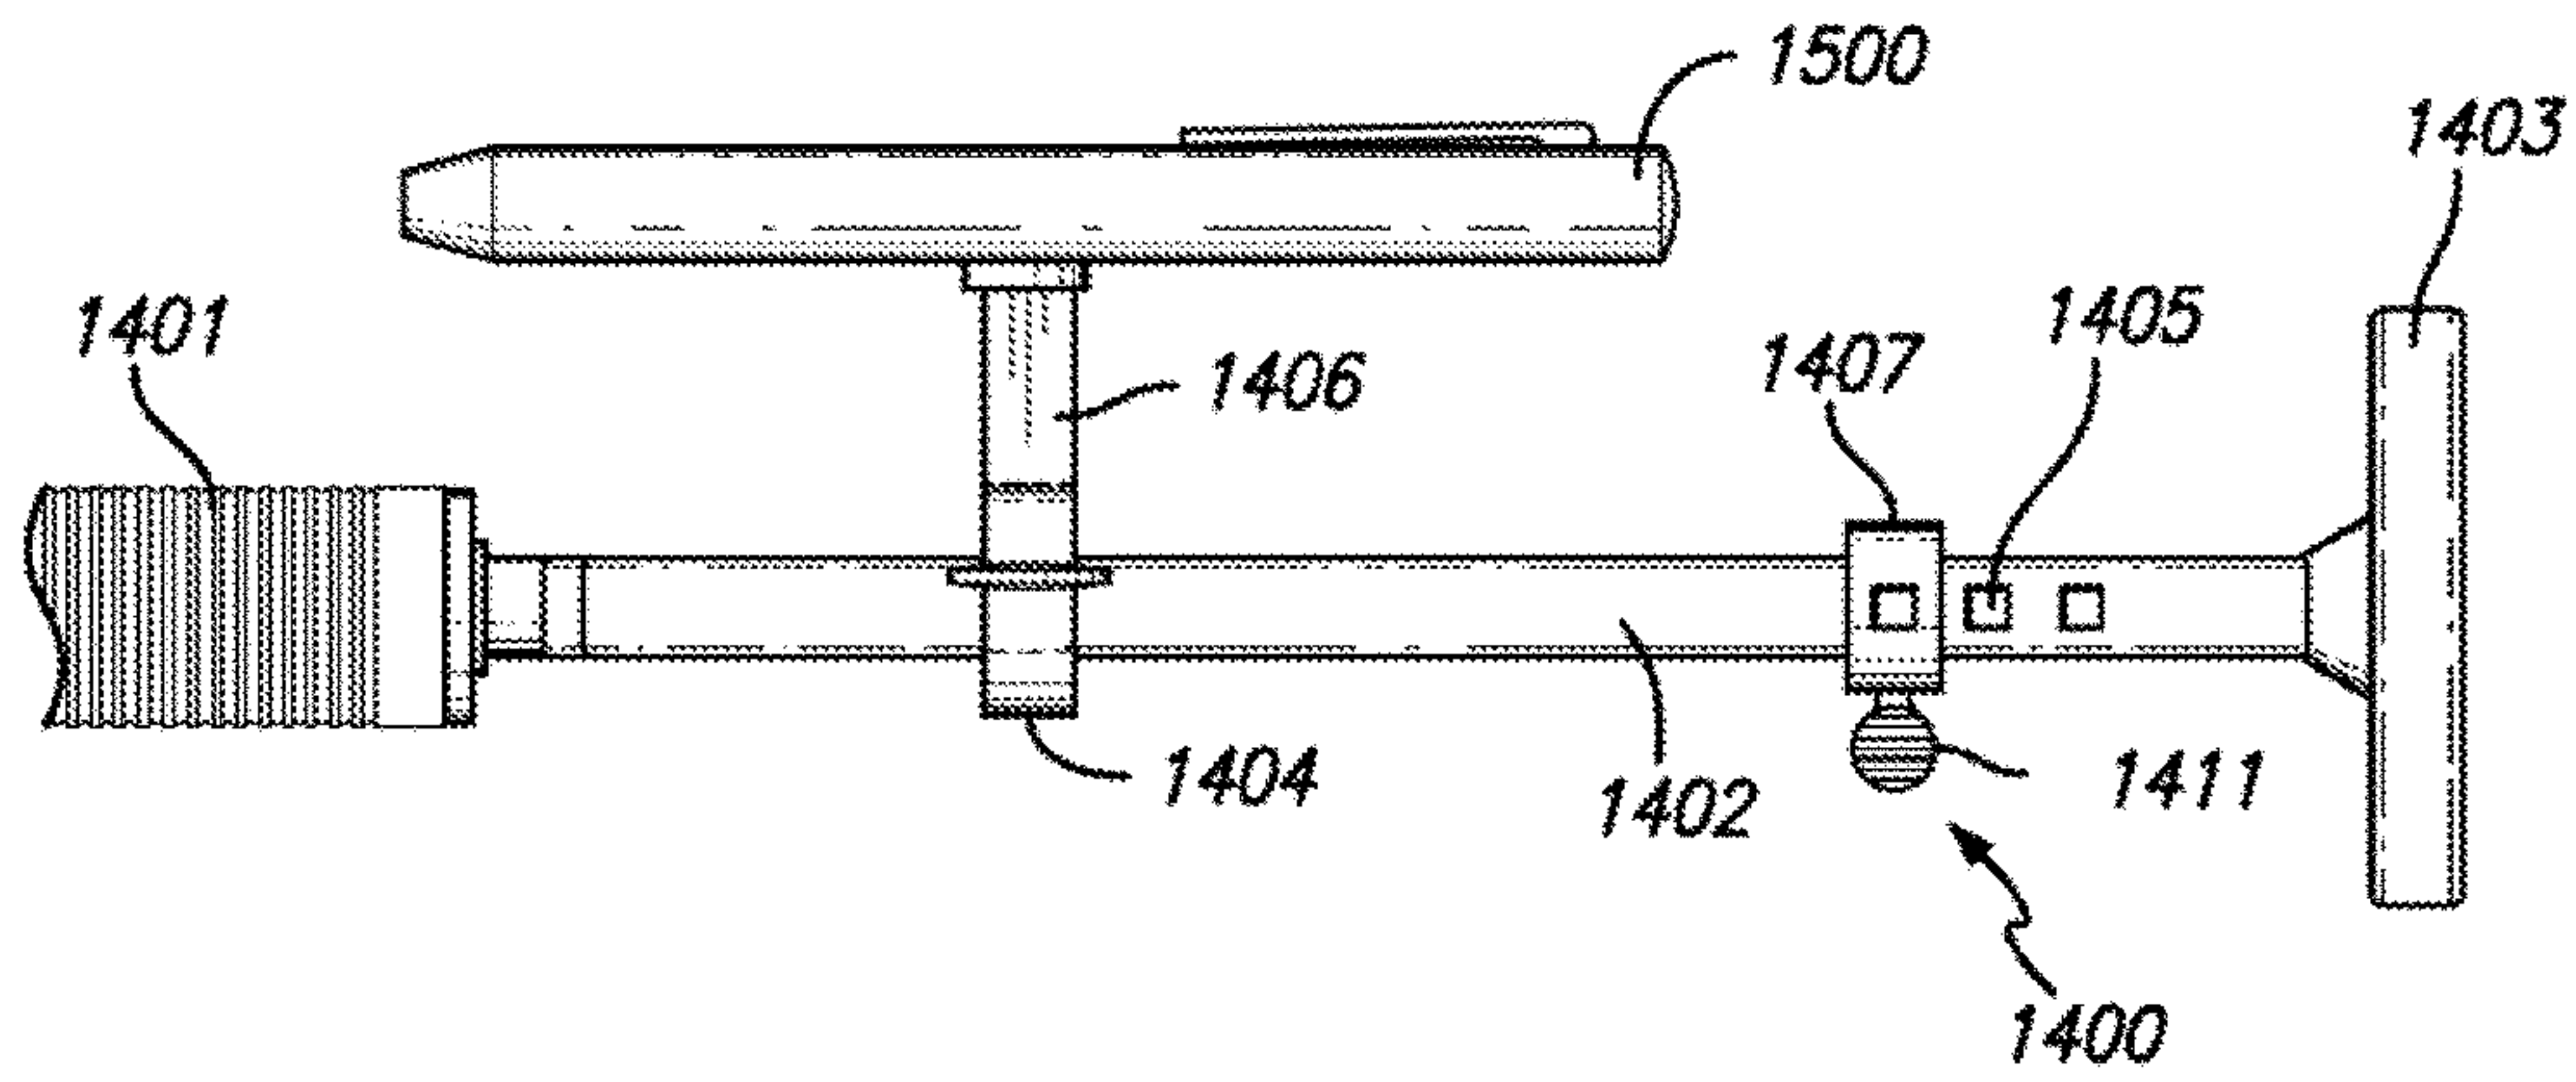


FIG. 19

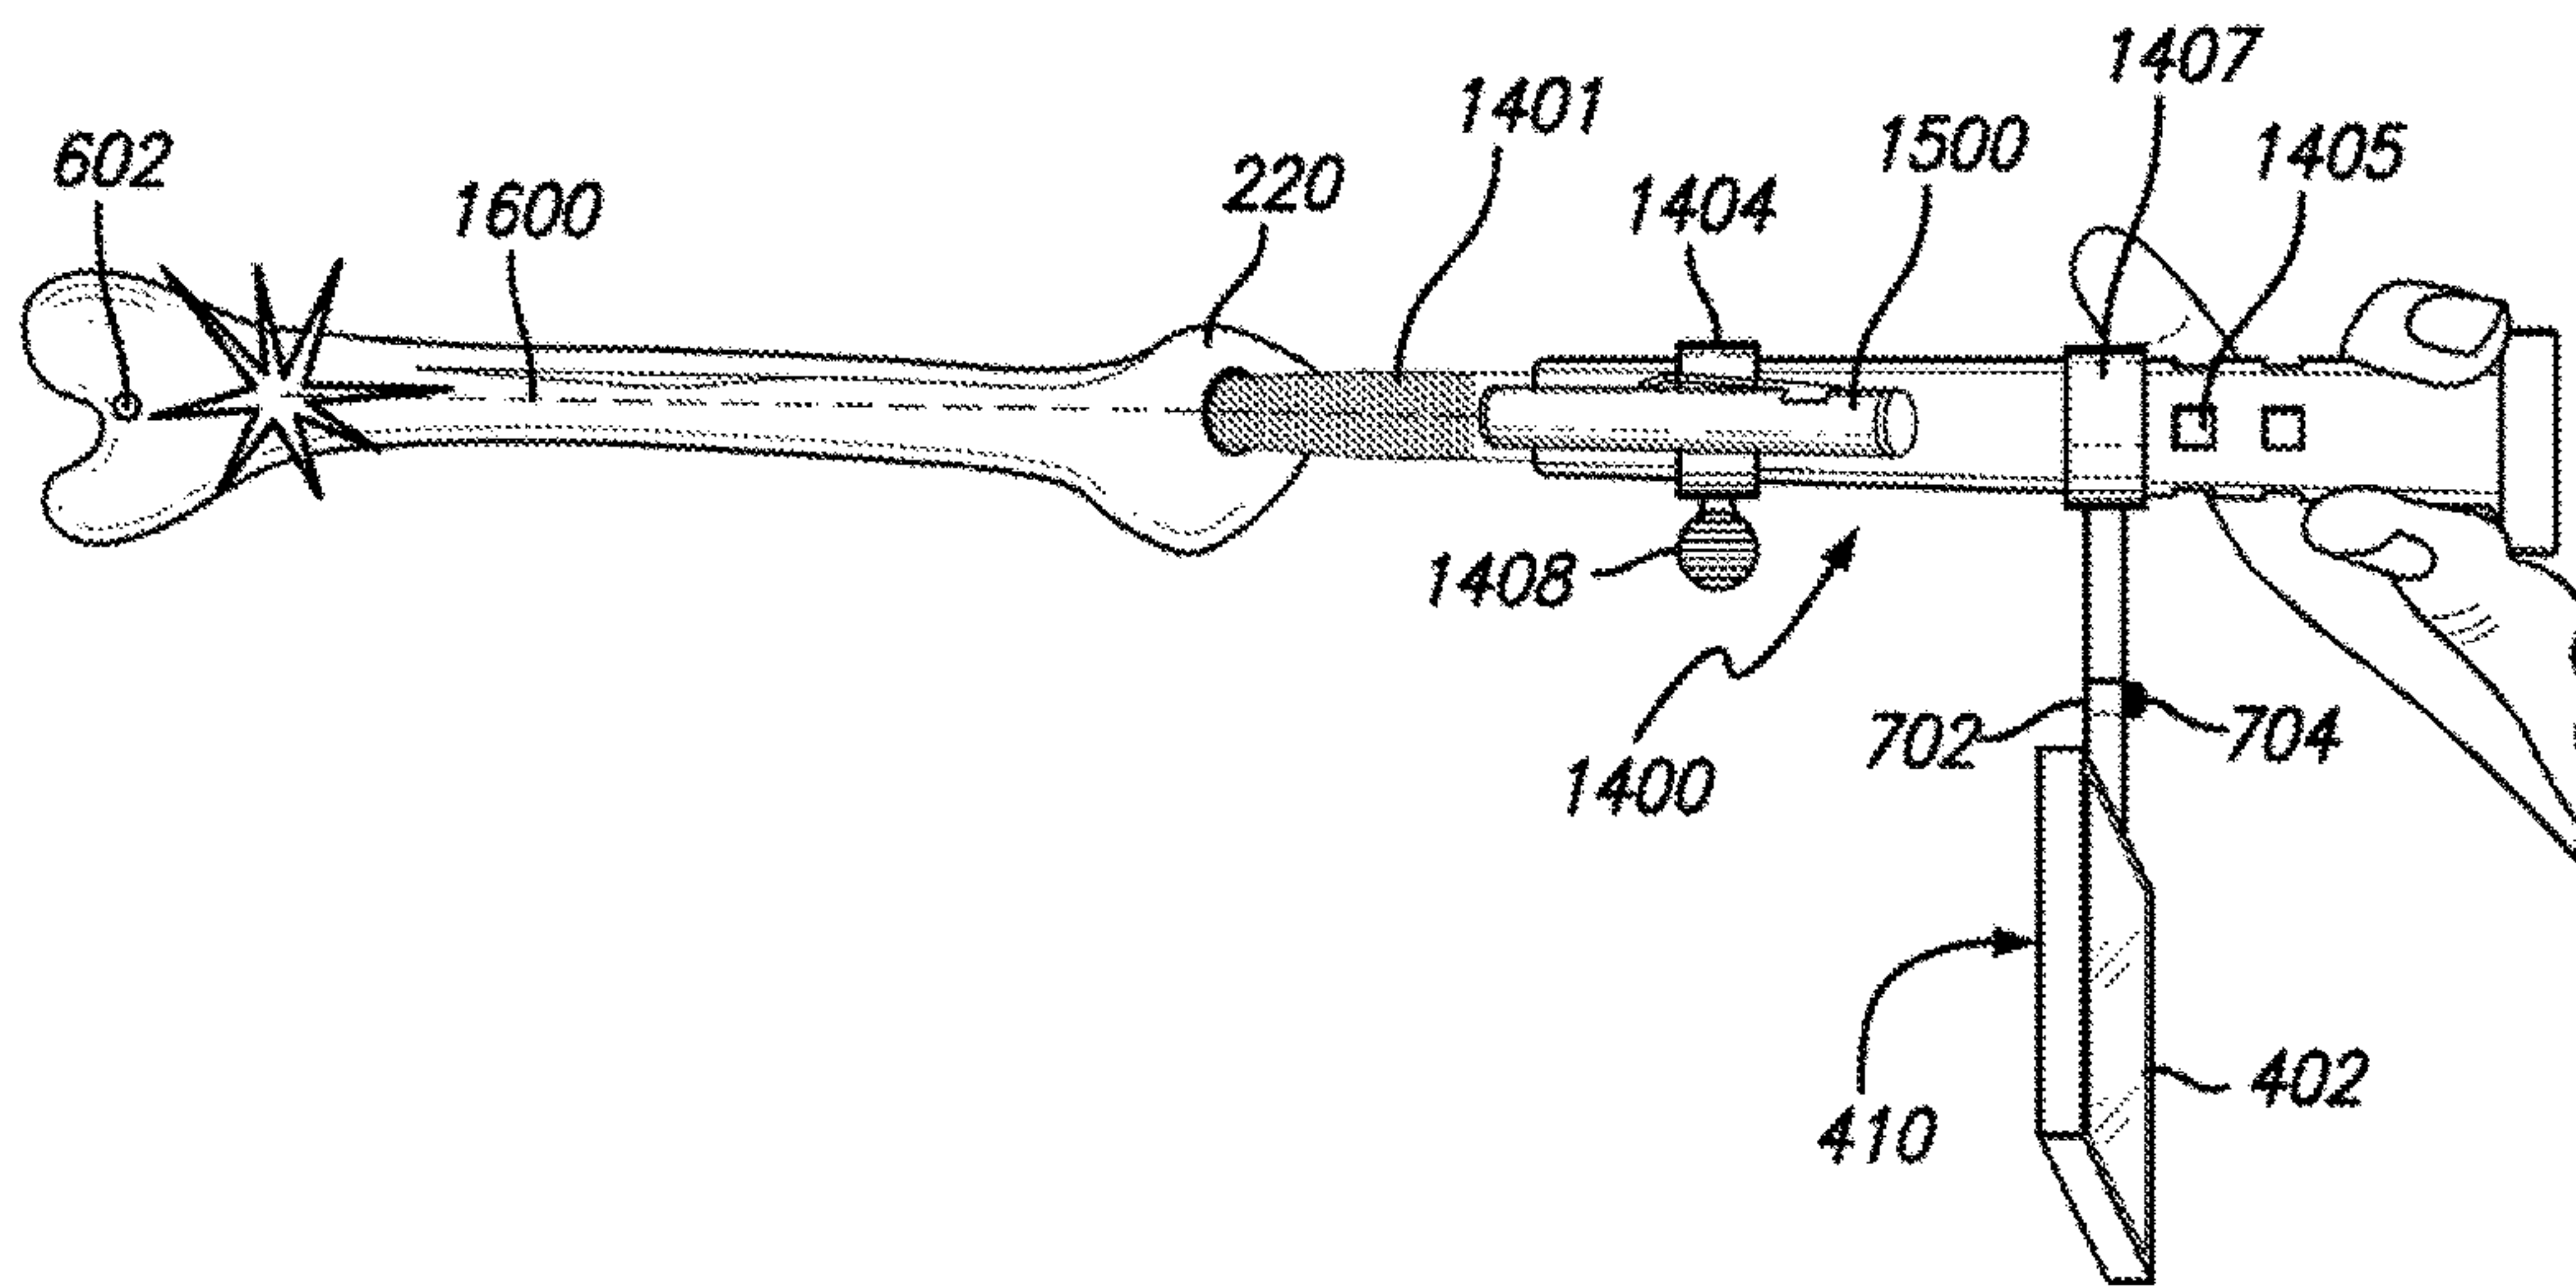


FIG. 20



## TELESCOPIC GUIDE FOR HIP REPLACEMENT METHOD

### CROSS-REFERENCES TO RELATED APPLICATIONS

This patent application is a continuation-in-part application of U.S. patent application Ser. No. 13/623,073, filed Sep. 19, 2012, which is a continuation-in-part application of U.S. patent application Ser. No. 13/440,962, filed Apr. 5, 2012, which is a continuation-in-part application of U.S. patent application Ser. No. 13/431,944, filed Mar. 27, 2012, which claims the benefit of U.S. Provisional Application No. 61/528,744, filed Aug. 29, 2011, and U.S. Provisional Patent Application No. 61/567,869, filed Dec. 7, 2011. All applications are incorporated herein by this reference thereto.

### BACKGROUND OF THE INVENTION

#### Field of the Invention

This invention relates to the field of minimally invasive surgical techniques for a joint replacement, and more particularly, methods for accurately positioning components for hip or knee joint replacement procedures.

#### Description of the Related Art

During the course of total hip arthroplasty, acetabular and femoral prostheses are placed. In order for the implants to function up to their capacity, generally meaning greater than twenty (20) years of clinical reliability, each component must be placed in a specific position in relation to the patient's native anatomy. Specifically, proper positioning of the acetabular component in a hip replacement procedure appears to be crucial to the long-term success of the surgery. What exactly constitutes proper positioning of the acetabular component is the subject of much debate. A commonly used range, established by Lewinnek et al., involves a cup position in which the abduction angle is within the range of 30° to 50° and in which the anteversion angle is within the range of 5° to 25°. Generally, surgeons use radiographic techniques to achieve these angles.

Studies have shown, however, that a substantially large percentage of surgeries result in cups that are not within this range. This is especially true with respect to minimally invasive surgical procedures. Callanan et al. surveyed 1952 hip replacements, observing several prediction factors, and found that only 48.7% resulted in acetabular cups within this range. Indeed, of the 93 hip replacements in Callanan's survey that used minimally invasive techniques, only 19.4% resulted in acetabular cups within this range.

This supports the proposition that traditional techniques have been considered by many to be unreliable for determining proper positioning of the acetabular cup or femoral component.

A variety of tools are available, however, to assist the surgeon in achieving correct component alignment. The so-called traditional guides, or line-of-sight, have been in use for over 40 years and are very helpful, but not as reliable as one would hope.

In the last 8-9 years, in an effort to improve reliability, there have been attempts at using so-called navigation or computer guidance systems relying on pre-operative CT scans to pre-load information pertaining to the patient's anatomy, intraoperative registration (a cumbersome and potentially tedious method to match the patient's anatomy to the preloaded image), the placement of multiple skeletal pins for orientation, and elaborate line-of-site transmitters relying on complex computer algorithms to guide compo-

nent placement. Unfortunately, in spite of the promise of improved results, the reluctance of patients to be exposed to a significant amount of radiation during a CT scan, the significant cost of such a test against a simple intraoperative x-ray treatment, the total cost of the computer guidance system (many hundreds of thousands of dollars plus the ongoing cost of support annually as the machine is maintained and updated), the incalculable cost to the healthcare system, and the patient of an unpredictable workflow as system breakdown occurs frequently, add operation time and potential risk to the patient, as well as considerable cost. Consequently, this method has not been widely adopted.

Furthermore, in spite of the existence of such tools, the current success rate for acetabular component positioning is only sixty percent (60%). Therefore, there is still a need to improve the reliability and efficiency of instrumentation in achieving these specific recognized optimal component positions.

### SUMMARY OF THE INVENTION

One embodiment of the present invention comprises methods for accurately positioning the acetabular cup in a minimally invasive, or conventional, total hip arthroplasty (THA), comprising the use of an elongated handle to place the cup in roughly the correct position with respect to the acetabulum of the patient, taking a first abduction reading and a first anteversion reading using a gyroscopic positioning unit aligned with the handle, taking an image of at least a portion of the cup using a radiography unit, using the image to determine the actual orientation of the cup and thereby the amount of movement in the abduction plane and in the anteversion plane to properly orient the acetabular component, incrementally altering the position of the cup by using a striking tool and an elongated instrument to tap a contact surface at one or more preformed impact receiving points, wherein the contact surface is in mechanical communication with the cup, taking new abduction and anteversion readings using the gyroscopic unit to determine the relative movement of the cup caused by the tapping, and repeating this striking step and this reading step until the cup has proper abduction and anteversion readings.

In another embodiment of the present invention, the surgeon may take additional intra-operative radiographic images during this process as needed. Other embodiments may also involve taking readings from a second gyroscopic unit aligned with a point on the pelvis so that any movement of the pelvis in any direction during surgery may be detected, quantified, and corrected. Such quantified movements are then used to adjust the target abduction and anteversion angles of the acetabular cup.

In some embodiments, a sterile surgical bag may be used to enclose the gyroscopic unit(s) to allow them to be situated within the operative field.

In further embodiments, employing the use of a portal incision remote from the main incision to permit precise acetabular bone preparation and cup implantation while employing a minimally invasive surgical approach, the proper placement of the portal incision is determined using an inside-out technique by using the geometry of the acetabulum to direct a path along a trajectory extending out from the plane formed by the face of the acetabulum to a point on the skin that provides perpendicular access to the acetabulum.

In some embodiments, a measuring tool may be used to precisely measure the proper location of the portal incision. In other embodiments, the measuring tool may be config-



ured in such a way that proper placement of the measuring tool inside the acetabulum positions the measuring tool to precisely guide a cutting tool to create a portal incision in the proper location.

To assist with proper femoral bone preparation and implantation, other embodiments may involve using a laser pointer or other positioning device to more accurately verify that the femoral broach is properly aligned with the femur while the surgeon is preparing the femur to receive the femoral prosthetic. The laser pointer may create a visible line or spot projecting generally parallel to the line of attack of the femoral broach. This permits more precise targeting of accepted anatomical landmarks such as the center of the popliteal space.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Some elements in the drawings have been drawn not to scale so that different features can be shown with better clarity.

FIG. 1 is a front view of an X-ray image of the pelvis showing acetabular components on both sides of a patient in a prescribed range of abduction angles as discussed above for long-term wear and joint stability in keeping with one embodiment of the present invention.

FIG. 2A is a perspective view of a tubular member in keeping with one embodiment of the present invention utilizing a directional device which is directed toward the center of the acetabulum, trial cup, or attachment end of an acetabular component placement tool, as discussed below, so that the directional device may reliably point the tubular member away from the acetabulum along a path that is generally perpendicular to the plane defined by the face of the acetabulum. The cutting member may thereby be directed through the tubular member and outward to the patient's skin where the portal incision will be made effectively at the optimal location, thereby creating access to the acetabulum along this path through the newly created portal incision.

FIG. 2B is a diagram of a tubular member in keeping with another embodiment in keeping with the present invention in which the turn radius is minimized to reduce the size of the cross-section necessary for the tubular member.

FIG. 2C is a perspective view of another embodiment of a tubular member that does not require a flexible tool.

FIG. 3A is a diagram of an embodiment showing the tubular member placed through a main incision in which the directional device assists the surgeon by pointing to the middle of the acetabulum (or trial cup, as discussed below, not shown). The cutting member thereby optimally takes a path generally perpendicular to the plane defined by the face of the acetabulum while allowing the surgeon to avoid critical blood. Note, the tissue such as nerves, tendons, ligaments, muscles, fat, and the like have been removed for clarity.

FIG. 3B is a diagram of another embodiment showing a tubular member in the vicinity of the pelvis bone and the acetabulum.

FIG. 4A is an embodiment of a measuring tool to facilitate creating a portal incision.

FIG. 4B is another embodiment of a measuring tool to facilitate creating a portal incision.

FIG. 4C is another embodiment of a measuring tool to facilitate creating a portal incision.

FIG. 4D is a close-up of the second end of the elongated member having a slot.

FIG. 5A is a diagram of an embodiment of the measuring tool in use to create a portal incision.

FIG. 5B is another embodiment of the measuring tool in use to create a portal incision.

FIG. 6 is a diagram of a trough in keeping with one embodiment in which a trough is used instead of or in conjunction with a cannula.

FIG. 7A is a perspective view of another acetabular component placement tool with a gyroscopic unit attached to the gyroscope holder in keeping with one embodiment of the present invention.

FIG. 7B is a drawing showing an acetabular component placement tool in keeping with one embodiment of the present invention inserted into the main incision with a cannula (to permit placement of, for example, an in-line impaction tool) resident in the portal incision. The side hole in the handle of the acetabular component tool is shown as round, but could readily be keyed or any other shape to ensure the proper orientation of the gyroscope holder that holds the gyroscopic unit.

FIG. 8 is a depiction of an acetabular component placement tool in use.

FIG. 9 is a drawing of the surgeon observing an image from a radiography unit in keeping with one embodiment of the present invention showing one preferred viewpoint of the radiography unit for use in combination with the gyroscopic unit in precisely positioning the acetabular component about two axes, the abduction angle and the anteversion angle.

FIG. 10A is a drawing of a strike plate in keeping with one embodiment of the present invention.

FIG. 10B is a drawing of a strike plate placed within a cavity of an acetabular component in keeping with one embodiment of the present invention.

FIG. 11 is a drawing of another embodiment of the strike plate showing a number of impact points to allow the selection of the appropriate locations on the strike plate for the surgeon to tap with a tapping instrument in order to achieve the desired movement of the acetabular component in situ as it engages the bone.

FIGS. 12A and 12B are diagrams of the relatively harder and relatively softer bone regions that the acetabular component encounters and that greatly add to the difficulty of precise placement and positioning of the acetabular component. These relatively hard and soft bone regions often cause the acetabular component to move in a complex path in reaction to the tapping described herein as part of one embodiment of the present invention. As a result, these hard and soft bone regions are one reason a strike plate having multiple impact points is particularly critical to achieving proper orientation of the acetabular component.

FIG. 13 is a perspective view of an embodiment of a disengagement tool to remove an impaction tool.

FIG. 14A is a drawing of a smartphone being used as the gyroscopic unit. It may have an open source or proprietary gyroscope application. The unit may then be placed in a sterile bag as shown for use during the surgical procedure.

FIG. 14B is a drawing of a smartphone gyroscopic unit in the sterile bag of FIG. 10 wherein the bag is stretched tightly and any excess is folded back and away from the screen so that the screen of the smartphone (or iPod or the like) remains readily visible to the surgeon and the touch-sensitive functionality of the screen remains accessible through the bag membrane.

FIG. 15 is a perspective view of a second gyroscopic unit fixed to a point on the patient's pelvis.



5

FIG. 16 is an image that may be produced by the combination of the positional data from the first and second gyroscopic units reflecting the position of the cup relative to the acetabulum and the plane defined by the face of the acetabulum during a hip replacement procedure in keeping with one embodiment of the present invention.

FIG. 17 is a perspective view of a femoral broach handle showing an adjustable mount for a pointer alignment device extending laterally from the handle that can allow adjustments for anteversion rotation of the broach and broach handle as it is inserted and to maintain a pointer directed precisely along the true posterior or true anterior surface of the femur. In keeping with one embodiment of the present invention, this alignment indicator—capable of indicating either or both of the broach longitudinal direction and anteversion orientation—reduces the risk of malposition of the femoral implant which can result in incorrect sizing or femur fracture.

FIG. 18 is another perspective view of the femoral broach handle of FIG. 17 in combination with a broach in place in keeping with one embodiment of the present invention.

FIG. 19 is a side view of the femoral broach handle with a laser pointer device attached in keeping with one embodiment of the present invention.

FIG. 20 is a perspective view of the femoral broach tool in use with a laser indicator light pointing toward the vicinity of the popliteal space and a gyroscopic unit to read the anteversion of the femoral broach in keeping with one embodiment of the present invention.

#### DESCRIPTION OF THE PREFERRED EMBODIMENTS

The detailed description set forth below in connection with the appended drawings is intended as a description of presently-preferred embodiments of the invention and is not intended to represent the only forms in which the present invention may be constructed and/or utilized. The description sets forth the functions and the sequence of steps for constructing and operating the invention in connection with the illustrated embodiments. However, it is to be understood that the same or equivalent functions and sequences may be accomplished by different embodiments that are also intended to be encompassed within the spirit and scope of the invention.

In general, minimally invasive techniques for total hip arthroplasty require making a main incision in the hip area of the patient to access the acetabulum of the pelvis, making a portal incision (described by this author in prior disclosures) to facilitate the proper positioning of an acetabular component, properly positioning the acetabular component in the acetabulum by making adjustments of the acetabular component through the main incision and the portal incision, utilizing the main incision to facilitate preparation of the femur to receive a femoral implant, and preparing the femur with a femoral broach to receive the ball that will be coupled with the acetabular component. One major goal is to achieve the proper abduction angle and anteversion angle as shown in FIG. 1.

One embodiment of the present invention involves an intraoperative system and method of locating the optimal position for the portal incision for a minimally invasive THA, properly positioning the acetabular cup, and properly preparing the femur. The portal incision in such an embodiment is located by making a main incision to access an acetabulum of a patient, using either a blunt or cutting member to forge a path through the patient's tissues along a

6

trajectory generally perpendicular to the plane defined by the face of the acetabulum, thereby identifying an appropriate portal incision location on the patient's skin while allowing the surgeon to avoid numerous blood vessels, muscles, tendons, and nerves in the process, making a portal incision at this identified point on the patient's skin. Then, the surgeon may use the direct, frontal access to the acetabulum created by this portal incision and path to prepare the acetabulum to receive an acetabular cup. This access may be further secured and maintained by using a cannula, trough or spatula device. In such instances, the surgeon may introduce the device to maintain the channel and thereby protect the contiguous tissues from additional injury by placing the device around the tip of the blunt or cutting member and then guide the trough-like device through the portal incision into the forged path.

In some embodiments, the acetabular component or cup may then be properly positioned to greatly improve the likelihood of success and longevity of the component, including attaching the acetabular cup to the end of an acetabular component placement tool and using the acetabular component placement tool to place the cup in roughly the correct position with respect to the pelvis of the patient. Knowing the approximate position of the patient's pelvis by virtue of the use of at least a semi-secure positioning device, the surgeon may then take a first abduction and a first anteversion reading using a gyroscopic positioning unit aligned with the acetabular component placement tool. The surgeon may then use a radiography unit to take an image of the pelvis containing the newly placed cup and use this image to more accurately determine the position of the cup.

In light of this true initial position, the surgeon may then alter the position of the cup incrementally by using a striking tool to tap a contact surface at one or more preformed impact receiving points, wherein the contact surface is in mechanical communication with the cup. The surgeon may take new abduction and anteversion readings to determine the how far the cup moved relative to the initial position due to the tapping, and then repeat the tapping and reading steps until the cup has reached a proper abduction angle and anteversion angle as indicated by the gyroscopic device display. The proper position for an acetabular cup is defined as a position in which the abduction and anteversion angles are within the predetermined acceptable ranges, as discussed above and widely researched in the literature.

This method indeed, among other benefits, allows the surgeon to properly position the cup without having to place any positioning pins in or on the patient, thereby avoiding the pain, risk of infection, and risk of pin movement that may accompany the use of positioning pin. This technique also eliminates the use of line of sight transmitters, e.g., RF type, which can be disrupted during the typical movements of personnel in and around the operative field, or by blood contacting the transmitters, or the computer crashing.

In some embodiments of the present invention, the femur may be prepared by a femoral broach mounted to a broach handle that involves a striking post and a straight-line pointer means. The means could be a light or laser pointer on an adjustable mount that is mounted on the handle to allow moving the pointer around, toward or away from, and/or along the handle or striking post. It can be locked into place once properly positioned to point along an optimal line, such as along the back of the patient's thigh generally toward or medial to the popliteal space of the knee. The surgeon then observes that the pointer continues to point at the chosen target in the direction of this chosen line while he or she repeatedly strikes the broach handle or striking post,



thereby ensuring that the femoral broach itself is properly oriented and aligned with the femur.

#### I. The Portal Incision

In one embodiment of the present invention, the surgeon locates the optimal position for the portal incision **244** by cutting from the inside out, or from within the main incision, along a trajectory away from the acetabulum **202** perpendicular to the plane defined by the face of the acetabulum. This technique allows the surgeon to locate a safe internal starting point and a safe path directed out to the under surface of the patient's skin better avoiding certain critical structures (veins, arteries, tendons, muscle, sciatic nerve, other nerves), forging a safe path or course around these structures while "sighting" or directing from inside or from within the main incision **242**. Then, once the starting location is identified adjacent to these critical structures as observed by the surgeon through the main incision **242**, a rigid, sharp or blunt or generally tubular body **100** is inserted adjacent to and without damaging these structures. The body **100** may be either curved as shown in FIGS. **2A** and **2C**, or angled as shown in FIG. **2B**. In some embodiments, the body **100** is generally tubular and a flexible tool **108** is passed through the hollow of the body and used to cut a path in the direction of the skin **240** distal to the main incision **242** to create an acetabular portal incision **244** from the inside out. In other embodiments, the body **100** itself has a sharp or blunt front end that may be used to cut or forge a path in the direction of the skin **240** distal to the main incision **242** to create an acetabular portal incision **244** from the inside out. In both scenarios, the path may be forged adjacent to and without damaging these critical structures in a manner best achieved in this inside-out method.

That is, by contrast, existing methods generally establish a location for the acetabular portal incision from visual cues or measurement made exclusively outside of the patient's body. With such outside-in methods, however, a trajectory is created and forged in which the surgeon cannot readily observe and avoid these critical structures in order to alter the path to accommodate variations in anatomy. These methods, therefore, typically cause the surgeon to risk encountering critical blood vessels, muscles, tendons, and nerves. Severing any of these can cause serious complications and unnecessary bleeding. Indeed, most outside-in methods lend to misjudging the proper location of the portal incision due to the inaccuracies in the rotational orientation of most common external visual guides. This error in rotation can even lead to perforating the femur anteriorly or piercing the sciatic nerve posteriorly. All of this may be avoided by the several inside-out methods described herein in keeping with the present invention.

In one embodiment of the present invention, therefore, a tubular body **100** is equipped on one end with a linear sighting or directional mechanism **104** to maintain a trajectory generally perpendicular to the plane P of the face of the acetabulum **202**. As shown in FIG. **2A**, in a preferred embodiment, the tubular body **100** is a hollow rod having a first portion **101** with a first opening **103**, a second portion **102** adjacent to the first portion **103**, the second portion **102** having a second opening **107** in communication with the first opening **103**, and a bend **109** connecting the first and second portions **101**, **102**. In other words, the first portion **101** bends into the second portion **102**.

The first portion **101** of the tubular body **100** is generally cylindrical and straight defining a first axis A and may serve as a handle. The first opening **103** may be positioned at or near the top or terminal end of the first portion **101** opposite the second portion **102**. In some embodiments, the first

opening **103** may be on the side surface of the first portion **101**. In some embodiments, the first opening **103** of the tubular body **100** may be on an auxiliary shaft **111** protruding outwardly from the first portion **101** at an acute angle. In some embodiments, the first portion may comprise multiple openings for the surgeon to choose from.

The second portion **102** allows the tubular body **100** to be properly positioned adjacent to the acetabulum in order to identify and create a path towards the location of the portal incision **244**. The second portion **102** comprises a lead **115** and a directional tool **104** coaxially aligned with the lead, the lead and the directional tool defining a second axis B. In some embodiments, the lead **115** comprises a second opening **107** perpendicular to the second axis B. Due to the bend **109**, the first axis A and the second axis B are non-parallel to each other. In some embodiments, the first axis A and the second axis B may form an acute angle with each other. In some embodiments, the angle between axis A and axis B is between  $25^\circ$  and  $75^\circ$ , in a preferred embodiment this angle is within the range of  $35^\circ$  and  $65^\circ$ . In some embodiments, the angle between axis A and axis B may be greater than  $90^\circ$  but less than  $180^\circ$  as shown in FIG. **2C**. This directs any tool traveling parallel to or along the second axis to move towards the surface of the skin **240** when the tubular body is properly placed in the main incision **242**.

In some embodiments, the bend **109** creates a tubular body **100** having an overall "J"-shape or hook-shape appearance as shown in FIGS. **2A** and **2C**. Due to the small amount of space afforded by the main incision in such surgeries, in some embodiments, the bend **109** may have a tighter curvature giving the external appearance of the tubular body more of a "T"-, "L"-, or "V"-shape as shown in FIG. **2B**.

That is, preferably, the main incision should be made as small as possible. Therefore, utilizing a tubular body **100** with a "tight" bend **109**, such as in the "V"-shaped embodiment in FIG. **2B**, would minimize the overall lateral dimensions, or width, of the tubular body **110**; thereby, allowing for a smaller main incision. With a "tight" bend, however, a flexible tool **118** may need to be particularly flexible to make the turn as easily as in a hook shaped bend. Therefore, the back wall of the bend **119** may instead have a rounded or curved shape, gradually turning away from the directional tool **114** and up toward the second opening **117** to guide the flexible tool **118** to make the turn at the bend **119** and proceed towards the second opening **117**.

The tubular body **100** may further comprise a directional tool **104** attached to the second portion **102** in a way that it defines a line of sight or a trajectory that is parallel to the second axis B. In other words, the lead **115** and the directional tool **104** are coaxially aligned. In some embodiments, the trajectory is along the second axis B as shown in FIGS. **2A** and **2B**. In another embodiment, the middle of the trial cup or the middle or the backside of the attachment portion of the acetabular component placement tool may comprise a feedback mechanism to facilitate this sighting by the directional tool **104** of the tubular body **100** and ensure that the tubular body **100** was in the correct position.

Alternatively, the directional tool **104** could be a laser pointing device, emitting a visible laser light **106** or the like. In some embodiments, the directional tool **104** may emit laser light **106** bidirectionally. For example, the directional tool **104** may be a cylindrical device emitting laser light **106** from both ends in opposite directions but along the same path. One end of the directional tool **104** could then emit a laser light **106** pointing to the middle of the acetabulum **202**, the middle of the trial cup that the surgeon may use for such positioning purposes, or the backside of the attachment



portion of the surgical tool **300** that attaches to the trial cup and holds it in place for such positioning purposes.

In such an embodiment, the opposite end of the directional device **104** would then emit a laser light **106** along the trajectory to illuminate a safe path to the portal incision **244** location. Alternatively, the safe path may be illuminated by a lighting device that is fed through the hollow of the tubular body **100**, such as an optical fiber or the like, and an imaging device may similarly be fed through the tubular body **100**.

In some embodiments, the directional tool **104** is configured to be removable from the tubular body **100**.

Due to the hollowness of the tubular body **100**, the tubular body **100** can receive a flexible tool **108** via the first opening **103** that can be fed through the first portion **101**, to the second portion **102**, and out the second opening **107**. Therefore, a diameter of the flexible tool **108** is smaller than a diameter of the first and second openings **103**, **107**. As the flexible tool **108** exits the second opening **107** it follows the path of the trajectory established by the directional tool **104** parallel to or along the second axis B. The flexible tool **108** may comprise a cutting instrument **150** at one end to cut through non-critical tissues or move aside the critical tissues to create a path towards the skin **240** where the portal incision **244** is to be made. In some embodiments, the flexible tool **108** may have a blunt end.

In addition, the flexible tool **108** may be a guide wire that traverses the path established by the trajectory towards the portal incision **244** while bypassing the critical tissue. A cannula, scoopula, sleeve, spatula, or similar guide tool **120** can be passed over or along the guide wire to maintain the path access to the acetabulum and/or to put the guide tool **120** in the proper position and orientation relative to the acetabulum for performing other techniques in the surgery without damaging critical tissue. In this embodiment, a cannulated, blunt, or sharp trocar, preferably approximately 8-10 mm in diameter, or other suitable tissue-protecting sleeve can be passed over this guide wire.

The flexible tool **108** can feed through the tubular body **100** and cut through the subcutaneous tissue and simply tent the skin **240**, thereby identifying the portal location **244**. While the skin **240** is tented, an apex is created and a 1-1.5 cm incision is made at this apex. Alternatively, still in keeping with the present invention, the surgeon may prefer to select a feed-through cutting member that is sharp enough and rigid enough such that the cutting member itself could actually cut through the skin at this optimal incision point **244**.

The cutting member **150** may then be fed through the skin a short distance. This tubular body can be proportioned so that a 4-12 inch cannula **121**, or a trough **120** as shown in FIGS. 3-5, can then be placed over its tip at a distance of about 1 cm (or enough to hold it in place) and the cannula **121** can then be led through the same safe soft tissue path thus avoiding veins, which in the common outside-in approach are typically severed and cause unnecessary bleeding. In such embodiments, the tip **124** or cutting member **150** of the flexible tool **108** may have a diameter that is slightly smaller than the diameter of the remainder or main body of the flexible tool **108** so that the junction where the main body transitions into the tip **124** defines a rim or ledge **122** extending radially outward from the outer surface of the tip **124**, as illustrated in FIG. 3A.

The flange or ledge **122** may be slight, approximately 0.5 mm, for example, and may be located about 1 inch or more or less from the free end of the tip **124**. The cannula **121** can be placed over the pointed tip **124** as it penetrates the skin **240** or otherwise passes through the portal incision until the

cannula or spatula reaches the ledge **122**. The sharp edges of the thin metal or plastic spatula or cannula **121** will thereby be covered as it is drawn through the soft tissue pathway defined by the flexible tool **108**.

In another embodiment, the working cannula can also simply be fed over a smooth trocar that is directed along the safe trajectory towards the skin. The skin is then tented, and an incision is made to permit the trocar to be accessible for mounting of and guidance of the cannula, spatula, or trough.

In yet another embodiment, the flexible tool **108** may be a thin-walled cannula or tissue-protecting sleeve, such as having a wall thickness of approximately 1-3 mm, an outer diameter of approximately 8-12 mm, and a length of roughly 10-40 cm. In this way, the cannula or trough member that maintains the just created path for use in preparing the acetabulum may be introduced from the inside out.

In some embodiments, the tubular member **100** is indeed not hollow but solid instead, as illustrated in FIG. 2C, having its own pointed or blunt tip **126** projecting from the lead **115** that may be used to forge the path along the generally perpendicular trajectory. The second end **102** of the member **100** may then have a ledge **128** between the lead **115** and the tip **126** that may then receive the end of the cannula or spatula member **120** and thereby act as a cannula introducer in a similar manner as discussed above. In some embodiments, the ledge **128** of the second end **102** may taper towards the tip **126**. In such an embodiment, the main body of the second end **102** may have a diameter that is slightly larger than a cannula, scoopula, spatula, sleeve, or similar type of guide tool **120** and the tip **126** may have a diameter that is smaller than any guide tool **120**. This allows any guide tool **120** to slip over the end **126** and stop where the opening of the guide tool **120** is substantially the same size as the diameter of the second end **102** (i.e., at the ledge **128**). In this sense, a single second end **102** can be used for different guide tools **120** having different sizes.

As mentioned above, the fixed trajectory created by the outside-in technique does not afford the surgeon with the opportunity to observe critical tissues and critical variations in anatomy or a misjudged anteversion orientation of an externally fixed sighting guide, all of which is avoided by the inside-out technique disclosed herein with reference to one embodiment of the present invention.

That is, this novel inside-out approach in this embodiment of the present invention allows the surgeon to actually see these vital structures from within and direct the potentially damaging hook or trocar through less vital tissues, such as fatty tissues, and particularly away from and around the vital structures and tissues. This visualization of the soft tissue environment can be additionally facilitated by optical fiber illumination and/or digital imaging of the environment to determine the alternative paths through the soft tissue along the trajectory generally perpendicular to the plane defined by the face of the acetabulum. In one embodiment, the illumination and imaging fibers can be passed through the cannulated hook. The fiber-optic light may also illuminate the skin from the inside out to indicate where to make the portal incision. The incision can be made on the brightest portion of the skin.

In some embodiments, the second portion **102** or **130** of the tubular body **100** or **110** may further comprise a joint or a hinge **112** or **125** to connect the first portion **101** to the second portion **102**. The hinge **112** or **125** allows the directional device **104** or **114** and the lead **115** or **127** (together defining axis B) to tilt in such a way so as to change the angle between axis A and axis B. The tilt of axis B relative to axis A may be controlled by a control mecha-



## 11

nism 113 or 129 to adjust the second portion 102 relative to the first portion 101. Preferably, the control mechanism 113 or 129 is a dial located at the top of first portion 101 or 132 of the tubular body 100 or 110 opposite the second portion 102 or 130. The control mechanism 113 or 129 may also have a locking mechanism (not shown) to lock the directional device 104 or 114 in place once the proper angle has been established. The locking mechanism may restrict or prohibit the movement of the control mechanism 113 or 129.

In other embodiments, the surgeon may tilt the first portion 101 or 132 of the tubular member during the procedure to manipulate the blunt or cutting end through the soft tissue and create the optimal path. In such embodiments, the surgeon may be able to continuously or periodically adjust the directional device 104 or 114 using the control mechanism to insure that the blunt or cutting end 150 continues to travel along the trajectory generally perpendicular to the face of the acetabulum.

The control mechanism 113 or 129 may utilize a connecting device (not shown), such as a flexible cable, rigid cable, rod, and the like, to operatively connect to the directional device 104 or 114, the lead 115 or 127, and/or the hinge 112 or 125. Movement of the control mechanism 113 or 129 can increase or decrease the length of the connecting device so as to cause the directional device 104 or 114 and the lead 115 or 127 to tilt. Use of the control mechanism 113 or 129 allows the surgeon to make very precise adjustments to the directional device 104 or 114 so as to point the directional device 104 or 114 to the center of the acetabulum 202 with minimal movement of the tubular body 100 or 110.

In some embodiments, the surgeon creates a portal incision 244 in the optimal location, without the need for marking the location prior to the incision, by utilizing a measuring tool 160 defining an axis D placed in a first position generally perpendicular to the main incision 242 to measure a distance from the acetabulum, and relying on that distance to measure an equidistant location, perpendicular to the axis D when in the first position, along the thigh. The measuring tool 160 contains a precisely angled slot 170 that directs the surgeon to the proper portal incision 244 location. This technique allows the surgeon to create a safe path directed towards the acetabulum while avoiding certain critical structures (veins, arteries, tendons, muscle, sciatic nerve, other nerves). By utilizing the measuring tool 160 and method of the present invention, a surgeon can reliably forge a path in which the surgeon can blindly but readily avoid these critical structures regardless of the variations in anatomy.

As shown in FIG. 4A, the measuring tool 160 for creating a portal incision 244 comprises a first elongated body 162 having a first end 164 and a second end 166 opposite the first end 164. The first elongated body 162 is generally straight or linear in shape, thereby, defining a first axis D through the first and second ends 164, 166 of the first elongated body 162. The first elongated body 162 may be graduated with a plurality of markings 168 evenly spaced apart on the body 162 along the first axis D.

A slot 170 may be positioned at the second end 166 of the body 162. The slot 170 is created by a recess on the surface of the first elongated body 162 defined by two parallel walls 172, 174 defining a slot axis S parallel to and midway in between the two parallel walls 172, 174. In the preferred embodiments, the slot axis S may form an approximately 45° angle X with the first axis D. Angle X defines the angle of entry for the cutting member 150 or the guide tool 120. Therefore, the slot 170 as defined by the two parallel walls 172, 174 and the top portion 176 and bottom portion 178 of

## 12

the body 162, when viewed from the side, has the appearance of a parallelogram having a center F along the slot axis S and midway between the top portion 176 and bottom portion 178 of the body 162.

In some embodiments, the measuring tool 160 may comprise a second elongated body 182 having a first end 184 and a second end 186 opposite the first end 184, the second body 182 defining a second axis E through the first and second ends 184, 186 of the second body 182. In the preferred embodiment, the length L2 of the second elongated body 182, from the first end 184 to the second end 186, is substantially the same as the length L1 of the first elongated body 162 as measured from the first end 164 of the first elongated body 162 to the center point F of the slot 170. The second elongated body 182 may also comprise a plurality of markings 188 evenly spaced apart on the second body 182 along the second axis E. The second end 186 of the second body 182 is connected to the first end 164 of the first elongated body 162 so that the first and second bodies 162, 182 generally form a right angle. Therefore, the slot axis S may also form an approximately 45° angle Y with the second axis E. In some embodiments, as shown in FIG. 4B, for example, the first and second elongated bodies 162, 182 may be fixed length.

Some embodiments may have a means for adjusting the first elongated body 162 relative to the second elongated body 182. Specifically, the first and second elongated bodies 162, 182 may be adjustable relative to each other such that the exposed or effective lengths L1 or L2 of one of the bodies 162 or 182, respectively, can be matched to the exposed or effective length L2 or L1 of the other body 182 or 162, respectively. For example, as shown in FIG. 4C, the first body 162 may comprise a series of arms 162a, 162b, 162c that are concentrically arranged with one arm 162c configured to slide into a second arm 162b, which in turn may be configured to slide into a third arm 162a, and so on. Similarly, the second body 182 may be n telescopic, being made of, for example, a series of arms 182a, 182b, 182c that are concentrically arranged with one arm 182c configured to slide into a second arm 182b, which in turn may be configured to slide into a third arm 182a, and so on.

In some embodiments, since the first and/or second bodies 162, 182 are intended to measure out discrete units, the exposed lengths L1, L2 of each arm 162a-c, 182a-c must be configured to be a factor of the base unit of measurement in between each marker 168 or 188. This will allow the measurements to be accurate when the first and second bodies 162, 182 are fully expanded or fully retracted. Exposed length L1, L2 refers to the portion of the first and second bodies 162, 182 that are visible and can be used in measuring.

In some embodiments, the resistance in between each arm 162a-c or 182a-c can be so tight that significant external force would be required to slide a first arm 162c or 182c into a second arm 162b or 182b so that the arms 162a-c or 182a-c would not move relative to each other just by adjusting the position of the first and second bodies 162, 182.

In some embodiments, a locking mechanism may be provided to fix the arms 162a-c or 182a-c in place to prevent unwanted sliding due to movement of the measuring tool 160. By way of example only, the locking mechanism may be a pin or ring that presses against the outer surface of the arms or is inserted into a hole in the arms. In some embodiments, one arm may have a dimple while the other corresponding arm may have a protrusion such that the protrusion can be seated into the dimple when one of the arms is extended to its desired position. In some embodi-



ments, a plurality of dimples and protrusions may be along the arms **162a-c**, **182a-c** so that that the arms **162a-c**, **182a-c** can be lengthened or shortened to discrete lengths. Any other mechanisms for reversibly fixing telescoping arms can be used.

In some embodiments, the first elongated body **162** may be slidably mounted on the second elongated body **182** so that the first elongated body **162** can slide up and down the second elongated body **182** along the second axis E. For example, the first end **164** of the first elongated body **162** may have a loop or collar that wraps around the second elongated body **182** so as to be adjustable relative to the first end **184** of the second elongated body **182** to change the length of L2. A locking member may be provided to lock the first elongated body **162** at the desired location. With the markings **188** on the second elongated body **182**, the surgeon can position the first elongated body **162** at any elevation above the acetabulum (i.e. the effective length L2 of the second elongated body **182**) and lock it in place. Knowing this elevation or effective length L2, the first elongated body **162** can be lengthened or shortened so that the effective length L1 of the first elongated body **162** as measured from the center F of the slot **170** to the first end **164** is the same distance as the elevation of the first elongated body **162** above the acetabulum (i.e. the effective length L2 of the second elongated body **182**). Variations of this arrangement can also be used, such as having the second elongated body **182** fixed or telescopic and the first elongated member **162** sliding horizontally perpendicular to the second axis E in which the entire elongated member **162** slides along the first axis D to adjust the distance of the second end **166** of the first elongated body **162** relative to the second end **186** of the second elongated member **182**.

In some embodiments, a hinge **190** may be used to connect the first elongated body **162** to the second elongated body **182** in an adjustable or foldable manner. This allows the measuring tool **160** to be stored easily particularly when combined with the telescopic embodiment.

In use during total hip arthroplasty, a main incision **242** is created on the hip lateral to an acetabulum **202**. Once the femur **220** has been removed, the measuring tool **160** may be inserted into the main incision **242** and abutted against the acetabulum **202** so as to define a first axis of measurement with the measuring tool **160**. A first measurement of a first distance from the acetabulum **202** to a first location outside the hip along the first axis of measurement may be taken. The measuring tool **160** is then removed from the main incision **242** and re-positioned with its first end **164** positioned at the first location and approximately perpendicular to the first axis of measurement within a coronal plane, such that the slot **170** is positioned at a second location a second distance away from the first location, so that the second distance and the first distance are equivalent in measure. A portal incision **244** can then be created by sliding a cutting member **150** or guide tool **120**, such as a spatula or cannula **121**, through the slot **170** towards the skin. The coronal plane is the plane dividing the patient's front half of the body from the patient's back half of the body, and for purposes of this invention, goes through the center of the acetabulum.

In embodiments in which the measuring tool **160** has two bodies **162**, **182** with fixed lengths, the surgeon makes a main incision **242** on the hip lateral to the acetabulum. The second body **182** of the measuring tool **160** is then inserted into the main incision and abutted against the acetabulum with the first body **162** generally outside and parallel to the hip within the coronal plane. Since the first and second bodies **162**, **182** are fixed relative to each other, the slot **170**

is automatically placed in the ideal location for creating a portal incision **244** if within the coronal plane. A cutting member **150** or guide tool **120**, such as a spatula or cannula **121**, can be slid through the slot **170** towards the hip to create the portal incision **244** without first requiring a marking.

In embodiments in which the measuring tool **160** has two adjustable bodies **162**, **182** connected at right angles, the surgeon makes a main incision **242** on the hip lateral to the acetabulum. The second elongated body **182** of the measuring tool **160** is then inserted into the main incision **242** with the first end **184** of the second elongated body **182** abutted against the acetabulum so as to define a first axis of measurement E with the second elongated body **182** and a second axis of measurement D with the first elongated body **162** that is generally outside and parallel to the hip. The second axis of measurement D may be generally perpendicular to the first axis of measurement E. With the second elongated body **182**, a first measurement of a first distance from the acetabulum to a first location outside the hip along the first axis of measurement E is taken. Alternatively, the effective length L2 of the second elongated body **182** or the elevation of the first elongated body **162** above the acetabulum may be first adjusted prior to taking the first measurement. With the first measurement in mind, the first elongated body **162** is positioned within a coronal plane through the acetabulum, and the effective length L1 of the first elongated body **162** is adjusted so that the slot **170** is positioned a second distance away from the first location that is equivalent in measure to the first distance. The portal incision **244** can then be created by sliding a cutting member **150** or guide tool **120**, such as a spatula or cannula **121**, through the slot **170** towards the hip.

Alternatively, the effective length L1 of the first elongated body **162** may be fixed. Therefore, the surgeon could simply insert the second elongated body **182** into the main incision against the acetabulum and adjust the effective length L2 of the second elongated body **182** until it matches the fixed effective length L1 of the first elongated body **162**.

Thus, the lengths of the first and/or second elongated bodies **162**, **182** can be adjusted for proper clearance from the patient, so long as the two bodies are adjusted to have equal effective lengths L1, L2.

In light of the above description, the distance of the path of travel P of the cutting member **150** or guide tool **120** is determined by the lengths L1, L2 of the elongated bodies **162**, **182**. In the preferred embodiment, since the elongated members **162**, **182** are at right angles to each other and the slot axis S, which determines the path of travel P, forms 45° angles with each of the elongated members **162**, **182**, the distance of the path of travel P can be determined the following equation:  $P^2=L1^2+L2^2$ . Therefore,  $P=\sqrt{L1^2+L2^2}$ .

In some instances, for example, when the hips are those of a patient who has suffered injury or deformation of the hips, the path of travel P may not necessarily form a 45° angle with the elongated members **162**, **182**. Nevertheless, since the elongated members **162**, **182** form a right angle with each other, the angle of entry X and the path of travel P can always be calculated since the lengths L1, L2 of the elongate members **162**, **182**, respectively, can always be determined using the above equation. In addition, the angle of entry X can be determined by using the equation:  $\tan X=L2/L1$ . Alternatively, once the path of travel P is determined, the angle of entry X can be determined by  $\sin X=L2/P$  or  $\cos X=L1/P$ .



In some embodiments, in order to change the angle of entry X, the slot 170 may be formed on a disc 192 attached to the second end 166 of the elongated member 162. The disc 192 is arranged so as to be rotatable within a plane defined by the elongated members 162, 182, and rotatable about an axis H perpendicular to the plane defined by the elongated members 162, 182. Pre-formed markings 194 may be placed on the disc 192 so as to determine the proper angle of the axis S relative to the elongated member 162. A marker 195 may be placed on the elongated member 162 to align with any of the preformed markings 194 to identify the angle of entry X.

In some embodiments, the disc 192 may be operatively connected to the first elongated member 162 in such a manner that adjusting the length L1 of the first elongated member 162 automatically adjusts the disc 192 so that the slot axis S is properly positioned to intersect with the tip of the first end 184 of the second elongated member 182. This can be done mechanically or electronically. Thus, when the first elongated member 162 is lengthened to increase L1, the disc 192 rotates clockwise to decrease the angle of entry X the precise amount so that the slot axis S continues to intersect the tip of the first end 184 of the second elongated member 182. Conversely, when the first elongated member 162 is shortened decrease L1, the disc 192 rotates counter-clockwise to increase the angle of entry X the precise amount so that the slot axis S continues to intersect the tip of the first end 184 of the second elongated member 102.

A locking member 196 may be provided to lock the disc 192 in place once the proper angle of entry X has been established. In one embodiment, the disc 192 may be rotatable on a backing 198 that is connected to the elongated member 162. The backing 198 may have a series of holes (not shown) along its periphery into which the locking member 196 can be inserted to lock the disk 192 in place once the proper angle of entry X has been established. Other types of locking mechanisms can be used.

## II. Positioning the Acetabular Component

As discussed above, proper positioning of the acetabular component 400 is critical for the prosthesis to function up to its capacity, but current methods are inaccurate, risky, and time-consuming. An acetabular component 400 may be any device designed to fit inside the acetabulum of a patient. By way of example only, an acetabular component 400 may comprise a cup, a trial cup, a reamer, a strike plate, and the like.

In one example, an acetabular component placement tool 300, such as the standard cup holder/alignment guide shown in FIGS. 7A and 7B, is commonly used in the medical profession to place and/or align the acetabular component 400 in the typical “best guess” position. Historically, because of the time consuming and technically challenging nature of obtaining an intraoperative x-ray, the true position of the component was not known until a recovery room, or office, x-ray was taken. The generally achieved success rate (achieving accurate positioning) is sixty percent (60%) (Rubash, et al.). Unless a very severe error was identified, nothing was done, and the patient carried the risk of early failure of the hip arthroplasty. If the cup position was too steep, then the plastic bearing surface could see excessive load and wear out prematurely, requiring corrective operation. If the angle was too shallow, then impingement of the femoral neck on the anterior rim of the acetabulum could result in dislocation.

Using the very recent advances in imaging technology, i.e., the availability of computer and or digital radiography, now makes it possible to obtain an accurate intraoperative

image within a few seconds, such as approximately ten (10) seconds, to approximately one hundred twenty (120) seconds. This image (film or fluoroscopic image, or possibly even CT or MRI) demonstrates the result of the “first try” or “best guess” position. Thus, in one embodiment, this image of the patient’s anatomy is used in conjunction with a gyroscopically enabled guide.

Having this intraoperative measurement, the surgeon now has an opportunity to make an immediate correction. At present, the sighting techniques with the traditional “best guess” instruments required one or more additional x-rays to confirm the correction. In addition, the traditional instruments were not constructed to permit careful, precise, known degrees of adjustment.

The present invention offers a new method and tool incorporating application for gyroscopic technology that provides a significant improvement when compared with the current sighting approach, i.e., sight, guess again, repeat the x-ray, and even possibly requiring that these steps be repeated again.

The present invention also eliminates significant cost, a critical factor in today’s health care system. There is no pre-operative CT scan, avoiding potentially damaging radiation exposure, especially in younger patients and particularly women of childbearing age. There is no upfront cost to the hospital in the form of capital investments of up to a million dollars or more, there is virtually no disruption of the desired workflow as the required intraoperative image can be obtained in under two minutes, interpreted in less than thirty seconds, and can be acted upon immediately thereafter.

In the preferred embodiment, a gyroscopic unit 402 may be placed in a sterile holder/container and affixed to a surgical tool 302, such as a straight or carefully angled cup holder/alignment guide, as illustrated in FIG. 7A. This upgrades the traditional directional device to a metered tool providing improved estimates during initial positioning of a prosthesis. An intra-operative radiographic image of the then-present position is achieved during initial estimated placement. The radiographic measurement is then used as part of the method for achieving successful positioning or the basis for making an intra-operative adjustment. Now, upon obtaining measurements from the gyrometer and an image from the intra-operative radiographic unit, the “best guess” positioning of the acetabular component 400 relative to the acetabulum 202 can be improved, the desired positioning can be determined and quantitated as to the correction required for proper placement of the acetabular component within the acetabulum.

In order to improve the accuracy, reduce the risk, and work efficiently, besides the proper positioning of the portal incision 244, some embodiments of the present invention utilize gyroscopes removably mounted on surgical tools 302 involved in acetabular component placement, referred to as an acetabular component placement tool 300, to provide a metered approach for adjusting the acetabular component in the acetabulum. Examples of surgical tools 302 that can be used in the present invention include, but are not limited to, a trial cup holder, a cup holder/alignment guide, an impaction tool, a reamer unit, and the like.

In general, an acetabular component placement tool 300 comprises a surgical tool 302 used in positioning the acetabular component 400, and a gyrometer or gyroscopic unit 402. The surgical tool 302 has a proximal end 304 connected to a distal end 306. The proximal end 304 is the end directly attached to or directly associated with the acetabular component 400. The distal end 306 is the end that



the surgeon can grasp to move the tool **302** in order to adjust the acetabular component **400**. The distal or upper end **306** may comprise a handle **308** to facilitate movement of the surgical tool **302**.

In the preferred embodiment, a gyroscope **402** may be attached to the distal end **306**. In some embodiments, the gyroscope **402** may be attached to the handle **308**. It is anticipated, based on the cost of gyroscopic technology, that only a nominal cost is required to add such a metering system, i.e., the “gyrometer,” to many existing surgical instruments with only minor modifications. Indeed, in some embodiments, a single gyroscope **402** may sense and display the angular orientation of the acetabular component **400** in two or all three of the traditional three (X, Y, and Z) planes. In other embodiments, two or three separate gyroscopes **402** may be employed to sense and indicate the angular orientation of the acetabular component **400** in each of the two or three orthogonal metered planes, separately. In this way, the surgeon can feel further assured that each sensor will most accurately detect the orientation or relative orientation within the chosen metered plane (e.g., the Y plane), exclusive of any movement in either of the two other planes (i.e., the X and Z planes).

In some embodiments, the gyroscope **402** may be integrally formed with the surgical tool **302**. In other embodiments, the gyroscope **402** may be removably mounted to the surgical tool **302** using a gyroscope holder **404**. The gyroscope holder **404** may be an elongated rod having a first end **408** that attaches to the surgical tool **302** and a second end **410** opposite the first end **408** that attaches to the gyroscope **402**. The surgical tool **302** may comprise a plurality of holes **406** at different levels. The holes **406** can be of any shape so long as the gyroscope holder **404** has a cross-sectional configuration keyed to fit into the holes **406** securely. For example, the holes **406** may be triangular, rectangular, hexagonal, star-shaped, circular with a notch, and the like. One end **408** of the gyroscope holder **404** would then have a cross-sectional shape corresponding to the shape of the hole **406** so as to fit tightly and securely into one of the holes **406** without being able to rotate. This allows the surgeon to attach a gyroscope **402** to the surgical tool **302** in such a way as to view the gyroscope readings. Adjustment of the holder, and thus the gyroscope, could also be carried out in order to facilitate a “zeroing effect,” creating a true read-out rather than a relative number.

In some embodiments, the gyroscope **402** may be incorporated in a conventional mobile electronic device **1000** containing a gyroscope **402**, such as a smart phone, iPod touch, iPhone, personal digital assistant, and the like as shown in FIGS. **14A** and **14B**. These common mobile electronic devices can be installed with an application for converting the yaw, pitch, and tilt or roll of the gyroscope **402** into the abduction and anteversion of the acetabular component **400**, and the tilt of the patient’s pelvis.

The gyroscopic unit **402** may be a gyrometer, inclinometer, accelerometer, magnetometer or compass, inertial sensor, GPS (Global Positioning System) unit, or an optical, infrared, or RF sensor. A gyroscope or gyrometer may be preferred in some embodiments in that such units often measure relative movement in two or three dimensions and in that many commercial devices have gyrometer units that can provide high-resolution measurements.

The gyroscope **402** can measure its relative position in three-dimensional space. Thus, any movement in the X, Y, and Z direction can be read by the gyroscope **402**. When the gyroscope **402** is attached to a tool or a patient’s hip or thigh, one or more reference angular readings of the tool or patient

in three-dimensional space may be communicated to the surgeon by the gyroscope **402** to monitor any movement of the patient’s pelvis. When associated with a smart phone or other computing device, the gyroscope **402** can display, announce, or otherwise indicate its relative position. The surgeon can set the initial position as the origin and calculate the amount of deviation from the origin necessary for correct positioning and move the surgical tool attached to the gyrometer **402** until the proper readings are reached. Alternatively, the correct positioning may be established as the origin and the gyrometer **402** may indicate the amount of deviation from the origin. Therefore, the gyrometer **402** can be moved until its readings reflect that it has reached the origin.

As mentioned above, in some embodiments, a gyroscopic unit **402** may be superior to a standard inclinometer or magnetometer. A standard inclinometer allows angular readings and correction relative to only the vertical axis. This single reading by itself cannot correctly position the acetabular component **400** to minimize wear and reduce risk of dislocation. Similarly, a magnetometer typically allows angular readings only relative to a near-linear magnetic field, such as the Earth’s magnetic field. The dual-axial or tri-axial reading from the gyroscopic unit **402**, by contrast, can inform the surgeon as to the relative movement of both the abduction angle (in a first plane) and the anteversion angle (in a second plane perpendicular to the first plane), as well as the tilt of the pelvis (in the third and remaining orthogonal plane).

Additional precision can be achieved if the pelvic tilt is controlled. The holder may also have a hinge **702** and set screw **704** so that the surgeon may “zero” the anteversion angle reading simply by adjusting the hinge **702** and then tightening down using the set screw **704** when the anteversion reading is just as the surgeon prefers. Examples of such hinge **702** and set screw **704** are illustrated in FIG. **7A**.

In the preferred embodiment, the gyroscopic unit **402** may be enclosed in a container **1002** to reduce and/or eliminate cross-contamination between the gyroscopic unit **402** and the patient. For example, the gyroscopic unit **402** may be wrapped inside a sterile bag. This also makes cleaning and reusing the gyroscopic unit **402** easy.

In yet another example that is still in keeping with some embodiments of the present invention, two or more gyroscopes **402**, **403** may be used for additional reference points to compensate for movement of the patient’s body, or the pelvis, rather than the movement of the acetabular component **400**. For example, a second gyrometer **403** may be used as a second reference point. The second gyrometer **403** may be mounted to a point on the patient’s anatomy, such as a point on the patient’s pelvis **200**, with a rod (not shown) or some other type of holder that would facilitate proper positioning of the acetabular component **400**. In some embodiments, the second gyrometer **403** may be attached directly to the patient’s anatomy without a rod, for example, with an adhesive that would still permit the surgeon to read the second gyrometer **403**. The direct attachment may be removable so as to remove the second gyrometer **403** when the surgery is complete. The surgeon may then be able to verify to what degree the patient’s pelvis **200** has moved since the initial readings were taken from both the first and second gyroscopes **402**, **403**. The surgeon may then use this degree of movement of the pelvis **200** to recalibrate the first gyrometer **402** or otherwise take such adjustments into account when calculating his or her target readings on the first gyrometer **402**, which, in combination with the readings from the second gyrometer **403**, is reflective of the position



of the acetabular component **400** in relation to the acetabulum **202** of the patient's pelvis **200**. In some embodiments, first and second gyrometers **402**, **403** may be in communication with each other so that the first gyrometer **402** receives the readings from the second gyrometer **403** and the first gyrometer **402** displays its readings regarding the positioning of the acetabular component **400** after compensating or adjusting for the movement of the pelvis as determined by the second gyrometer **403**.

In some embodiments, the two gyrometers **402**, **403** may communicate with each other or with a local computer **800** so that the changes in target readings of the first gyrometer **402** (i.e., the target position of the prosthetic cup) may be tracked, communicated, and even displayed on a monitor **802** to indicate to the surgeon how the patient's pelvis may shift during the procedure. As shown in FIG. **16**, computer software can transform the readings and radiographic image of the actual, relative orientation of the acetabulum **202** and acetabular component **400** into a two- or three-dimensional image representation of the cup **300'**; acetabulum **202'**; and plane **203'** defined by the face of the acetabulum combination and display it on a screen **802** either on one of the gyrometer units **402**, **403** or on the local computer **800** in real time so that the surgeon may get a good sense of how the acetabular component **400** is located and moving relative to the acetabulum **202** during the procedure as the surgeon moves the acetabular component **400** in at least two dimensions relative to the acetabulum **202** (i.e., in the abduction and in the anteversion directions) and as the patient's acetabulum **202** itself may move in any direction during the procedure.

In some embodiments, instead of, or in addition to, displaying the readings of the gyrometer **402**, the gyrometer **402** may announce the readings orally, or use a tone or some other aural indicator, so that the surgeon does not have to take his eyes of the patient to read the gyrometer **402**. The gyrometer **402** can announce either the current location so the surgeon knows where he needs to move the acetabular component **400**, or the gyrometer **402** can announce the type of movements the surgeon needs to make to properly position the acetabular component **400**.

Minor adjustments may be made with an impaction tool **600**, such as a strike plate as shown in FIGS. **10A**, **10B**, and **11**. An impaction tool **600** is configured to protect the acetabular component **400** as the acetabular component is being struck for proper positioning. In some embodiments, the impaction tool **600** may comprise multiple striking ports **700**, such as corrugations, dimples, depressions, divots, recesses, and the like impaction surface on the inside **602**. The outside surface (not shown) of the impaction tool **600** contacts the inside of the acetabular component **400** and creates a high-friction contact. Due to the high friction, movement of the impaction tool **600** causes movement of the acetabular component **400**. Therefore, small increments of precise adjustment of the acetabular component **400** can be made by tapping on the impaction tool **600** without damaging the acetabular component **400**. Such precise and incremental movements are critical, particularly because of the combination of hard and soft bone surfaces that the acetabular component **400** must engage with and seat into. The impaction tool **400** also, in some embodiments, may have regions through which the surgeon may see through to the bone to confirm that the cup is fully seated.

In some embodiments, the impaction tool **600** may be a total contact shell mating with the inner concavity of the acetabular component **400** and secured via a central screw. The exposed surface of this shell presents multiple striking

ports **700** on the inner face **602** to assist with fine adjustments of abduction or anteversion as the acetabular component **400** is seated. The surgeon may alternately strike the off center ports **700** and then the central port, depending upon the changing position of the prosthesis as it is seated. It is important to appreciate that the bone density typically varies around the rim, along the walls and at the dome of the prepared acetabulum as shown in FIGS. **12A** and **12B**. For example, the acetabulum may have hard areas **900** and soft areas **902**. Because of this variability, the prosthesis, if not monitored and controlled as it is seating, will follow the course of least resistance. Following that course creates a high risk of component malposition. Traditional positioners provide only for a central striking surface and a handle to generate a rotational force at a point removed from the implant itself and therefore not as precise as needed. The latter, central striking only technique, typically requires disengagement and re-engagement as the cup approaches final seating. This allows for the possibility of losing some pressfit as the bone is compressed with the first seating and then can lose some "stiction friction" or press fit upon reseating into the newly compressed bone.

In some embodiments, the impaction tool **600** may further comprise a flange **608** at the opening of the impaction tool **600**. The flange **608** can be one continuous ring around the open edge of the impaction tool **600** parallel to and in the plane of the strike plate opening. Alternatively, the flange **608** may be short segmented flanges intermittently spaced apart around the edge of the opening. These flanges **608** can further serve as striking points to permit greater angular momentum for moving the actual acetabular component **400**. In some embodiments, the flanges **608** may comprise striking ports **700**, such as dimples, recesses, divots, depressions, corrugations, or other modifications to facilitate striking of the impaction tool **600**. The striking elements in all cases are situated and construed in a manner that protects the surfaces of the acetabular prosthesis.

In some embodiments, the surgeon may tap the flange **608** with the impaction tool **600** while the elongated handle remains attached to the acetabular component. In other embodiments, the surgeon may remove the elongated handle so that the surgeon may have numerous other striking ports **700** to select to tap with a striking tool (not shown). In such an embodiment, the strike plate or acetabular component **400** can have a keying surface, such as one or more component keying features **605**, so that the surgeon may quickly and easily re-seat the elongated handle within the acetabular component **202** from time to time to take new abduction and anteversion readings from the gyroscope **402**.

For example, the component **202** may also be keyed, such as with one or more matching keying members **405**, to mate with the keying surface of the impaction tool **600** in order to re-seat the proximal end **304** of the tool **300** in an identical orientation. The gyrometer holder may also be keyed in order to re-seat it in an identical orientation.

In some embodiments, a disengagement tool **1300** is provided for the surgeon in case the acetabular component is so firmly impacted that simply striking off center will not result in the desired repositioning and may get stuck in the hard and soft bone material **900**, **902**. That is, surgeons may find the cup or other component may get stuck or frozen within the acetabulum making it difficult or nearly impossible to adjust the component any further. The surgeon may then use the disengagement tool **1300** shown in FIG. **13** to carefully and minimally, in a controlled manner, pry the component, such as the impaction tool **600**, loose so that he or she may then re-institute the routine described above in a



## 21

further attempt to properly position the component using the radiographic unit and/or the gyroscopes.

The disengagement tool **1300** may comprise a handle **1302** and an arm **1304** attached to the handle **1302**. At the end opposite the handle **1302**, the arm **1304** may branch or fork into multiple prongs. The impaction tool **600** may comprise a plurality of fenestrations **604**. A first prong **1306** may be configured to engage a first fenestration. A second prong **1308** may be bent at an angle relative to the arm **1304** and/or the first prong **1306** so as to engage a second fenestration. In some embodiments, the first and second prongs **1306**, **1308** may be configured so that the first prong **1306** can engage the first fenestration while at the same time the second prong **1308** is able to engage a second fenestration. This can improve the leverage of the disengagement tool **1300** to more easily remove the impaction tool **600**. To further improve the leverage, additional prongs may be added, one or more of the prongs may be adjustable or extendable to accommodate a number of feature configurations on the accessible surface of the impaction tool **600**. In some embodiments, the disengagement tool **1300** may be configured to engage the striking ports **700** to remove the impaction tool **600**.

The handle **1302** may be any shape. In some embodiments, the handle **1302** may be planar. A planar surface could provide a striking surface to controllably move or remove the impaction tool **600**. In some embodiments, the handle **1302** may comprise contours so as to be ergonomically shaped to facilitate grasping of the handle **1302**.

## EXAMPLE 1

Generally, when using an acetabular component placement tool **300**, start with the “Best Guess” approach (using the traditional “Sighting” Guide approach, plus the Cup Holder/Alignment Guide), obtain a radiographic or fluoroscopic image, and then use one embodiment of the present invention to make precise adjustments.

For example, once all of the proper incisions have been made and the acetabular component **400** is initially put in place with an acetabular component placement tool **300**, the present settings of abduction and anteversion are read from the gyroscopic device **402**. An imaging device **804**, such as those used in radiographic or fluoroscopic imaging, can be used to create a radiographic or fluoroscopic image. For example, the imaging device **804** may be an x-ray machine emitting x-rays **806**. From the radiographic imaging, the degree of abduction and anteversion needed for proper placement of the acetabular component **400** can be determined. Then, as the acetabular component placement tool **300** is shifted in the desired direction(s), the gyroscopic device **400** displays the real time changes in degrees so that the surgeon knows how much movement has been made, and how much more movement in a particular direction is still required. This reading, in reference to the starting position, gives the surgeon precise affirmation that the ideal position for stability and durability has been achieved.

The application of the gyroscopic indicator offers a reading, a numerical equivalent, that records the position in space that corresponds to the instant positioning confirmed on x-ray. The correction can then be made. Precise adjustments in the two critical planes (abduction and anteversion) can now be guided by observing the gyroscopic readout. For example, the readout can be calibrated to the amount of correction desired in each plane and noted to be correct when reading zero for abduction and anteversion. Another embodiment would be to set the gyroscope at the measured

## 22

abduction and anteversion and simply correct or change the component position to the desired reading which would then indicate the desired position has been achieved.

## EXAMPLE 2

In yet another embodiment, the best guess position can be made more precise by applying the present invention to the standard cup holder/alignment guide and, rather than relying on line of sight, i.e., identifying a neutral or zeroing orientation that at present is simply “sighted” in relation to operating room structures (a corner of the room, a vertical line of tiles on the wall, or any nearby straight vertical object) or imprecise anatomical landmarks (patient’s trunk, shoulder, opposite kidney). That is to say, that the gyroscopic indicator is capable of indicating true vertical for the upright part of the guide and true zero or neutral for anteversion. After cup placement in the orientation directed by the combined references of the present invention connected (physically or remotely) to the recently redesigned alignment guide, the guide is then removed. Screws or a trial liner may then be placed. A femoral trial may also be placed in the best guess position either before or after placing the acetabular component. An x-ray or fluoroscopic image is then obtained.

Those “corrected numerical” readings are used when placing the actual acetabular component. The instrumented portion of the reamer handle can then be transferred to the standard alignment guide.

## EXAMPLE 3

This example is similar to Example 1 above, but including an attached **35** “gyrometer.” The reamer basket (not shown) itself can act as a surrogate for the acetabular component **400**. The gyrometer **402** settings can then be noted, an x-ray taken, and any corrections identified by measuring angles on the x-ray. This could be considered a way of calibrating the gyrometer **402**. When returned to the same position (as indicated by the subsequent gyrometer **402** readout), correct acetabular component **400** positioning is then achieved by placing the acetabular component **400** in position, which results in corrected gyrometer readings.

By using a digital gyroscopic unit, the surgeon can quantify the orientation in space of the acetabular component greatly improving on the “best guess” orientation in which the surgeon might otherwise eyeball the positioning. Clinical research to date (including, Rubash, et al.) confirms a 40% error rate with current “best guess” in which the surgeon does not use such digital sighting or directional instruments.

The combination may create an advantage, including by avoiding the need for the unreliable “line of sight” relative referencing or the booting and rebooting of a computer, both of which take substantial time and have been cumbersome and unreliable. Indeed, these cumbersome and unreliable techniques have been abandoned at many centers. As stated, forty percent (40%) of the time, the position will be outside of the desired range and a correction will be desirable. The data indicates that the success rate using the intraoperative imaging and adjustment methods of the present invention can be improved from sixty percent (60%) to almost ninety-nine percent (99%)—and this significant success rate may be produced using minimally invasive surgery procedures.

Some embodiments of the present invention also may eliminate the need for reference pins in the pelvis as such pins can loosen, change position, and diminish precision.



The pin sites can become infected and require treatment with costly and risky antibiotics. A persistent pin site infection could result in migration of bacteria to the new prosthesis with disastrous results. While placing pins there is risk to nearby nerves and blood vessels. Numbness, weakness, or unnecessary blood loss could occur. There is also a price to pay in terms of time and materials. Clearly, avoiding reference pins offers a significant advantage.

### III. Positioning the Femoral Broach

In some embodiments of the present invention, the femur **220** is prepared by a femoral broach tool comprising a femoral broach **1401**. The femoral broach **1401** may be mounted to a broach handle **1400**, which comprises an elongated connecting member **1402**. A striking post **1403** then may be connected either to the connecting member **1402** or directly to a portion of the femoral broach **1401** to allow the surgeon to strike the striking post repeatedly until he or she has displaced the appropriate amount of bone material from the femur to leave room for the prosthesis and any associated mounting structures and cementing material.

The lengthwise orientation of the femoral broach **1401** during this process is critical to the successful preparation of the femur **220** and ultimate positioning of the prosthesis. In previous methods, the surgeon lined up either the connecting member **1402**, the striking post **1403**, or the hammer itself with line of sight methods previously disclosed by Applicant in considerable detail. In short, this often entails envisioning the femoral broach **1401** to be in line with the striking post **1403** and attempting to keep the striking post **1403** therefore in line or parallel to some straight line along the patient's leg or other straight line in the operating room that serves as a proxy to the centerline of the patient's femur **220**.

As shown in FIGS. **17** through **20**, another aspect of the present invention is the femoral broach handle **1400** being equipped with a more precise alignment means to visibly align the femoral broach **1401** during the bone displacement. The femoral broach handle **1400** comprises an elongated connecting member **1402** defining a central axis **C** (which defines the line of attack), attached to a striking surface, platform, or post **1403**, to hold and drive the femoral broach **1401** into the femur, and an adjustable mount **1404**. The adjustable mount **1404** is connected to the connecting member **1402** in such a way as to allow the adjustable mount **1404** to rotate about the connecting member **1402** as well as slide up and down the connecting member **1402**.

The adjustable mount **1404** comprises a post **1406** and a lock **1408** to receive and secure a pointing device **1500**, such as a laser pointer. The post **1406** may also be telescopic to adjust the distance of the pointing device **1500** relative to the connecting member **1402**. Due to the adjustable mount **1404**, the laser pointer **1500** may be offset from the central axis **C** of the femoral broach **1401** and connecting member **1402**, and it is oriented to emit a light or laser generally parallel to this central axis **C**. In some embodiments, the surgeon then can adjust the positioning of the pointer **1500** so that the light emitted from it runs along the back of the thigh approximately toward the popliteal space **602**, strikes the back of the thigh near the region of the popliteal space **602**, strikes the back of the calf just past the region of the popliteal space **602**, or strikes any other desired precise reference point that guides broach and the prosthesis orientation.

The mount **1404** for the pointer **1500** may be adjustable in a number of ways relative to the connecting member **1402** to accommodate the surgical procedure. In one such embodiment, for example, the mount **1404** may be a collar rotatably mounted to the connecting member **1402**, such that it can be

rotated about the central axis **C** of the connecting member **1402**. The surgeon may simply rotate the offset mounting arm about the central axis **C** of the connecting member **1402** and then fix the pointer at an appropriate angle using the lock **1408**, such as a set screw or the like, to indicate the anteversion angle as the broach seeks the desired neutral position in the femoral canal. The mount **1404** may also be slideable along the connecting member **1402** so as to adjust the distance from the broach **1401**. The mount **1404** may also have a tilting capability to allow the laser pointer **1500** to be adjusted so as to be parallel to the connecting member **1402**.

In this way, the pointer **1500** may be adjusted to visibly maintain the central axis **C** in any preferred anteversion angle, regardless of the anteversion angle of the handle **1400** so that the surgeon can project the laser light **1600** directly over the posterior or anterior femur while orienting the broach **1401** in the same or any other desired anteversion angle. The surgeon then observes that the pointer **1500** continues to point at the chosen target in the direction of this central axis **C** of the connecting member **1402** as he or she repeatedly strikes the striking post **1403** or surface of the broach handle, thereby being certain that the central axis **C** of broach **1401** itself is properly oriented and aligned with the central axis of the femur.

In one preferred embodiment, therefore, the anteversion angle of the femoral broach may be monitored, and in fact a gyroscopic unit **402** may be mounted to the broach handle **1400** in a similar fashion as discussed above with respect to the handle **1400** for the acetabular component **200**. As illustrated in FIG. **20**, there may be a mounting arm **1407** having a lock **1411** as well as a pivot means **702** and locking means **704** so that the anteversion of the broach may be zeroed intraoperatively. Furthermore, a second gyroscopic unit **403** may be temporarily mounted to the patient's body, such as the thigh or knee region, as a reference reading to assist with a precise anteversion reading for the broach **1401** even if the patient's leg happens to move or shift during the procedure.

This is especially important when placing a cemented implant that is not guided by the prepared bone envelope. That is, the handle and alignment means may hold the femoral component in the proper longitudinal alignment while the cement sets so that any forces on the femoral component as the cement begins to set may be overcome by the surgeon. The surgeon may additionally wish to maintain a given anteversion angle for the femoral component using the same handle and alignment means.

Whether employed in the setting of the femoral prosthesis or not, the anteversion readings for the femoral broach and/or prosthesis itself can be used to calculate or modify the target anteversion range for the acetabular component **200** unique for the given patient. That is, the anteversion angle for the femoral component can fall within a wide range, ordinarily between  $0^\circ$  and  $70^\circ$ , and typically is dictated by the contours of the patient's femur. This may be due to a number of factors unique to each patient. As a general rule, therefore, the anteversion angle of the acetabular component normally is more easily varied than the anteversion angle of the femoral component.

The actual angle of anteversion of the femoral component for most patients can affect what is the appropriate target range for the anteversion angle of the acetabular component for a hip replacement to have a successful longevity. Typically, the larger the anteversion angle of the femoral component, the larger the anteversion angle needs to be for the acetabular component, leading to increasing the target



25

acetabular anteversion angle to within a range of 20 to 25, where the patient's femoral anteversion angle is on the higher end of the above-mentioned range.

While the present invention has been described with regards to particular embodiments, it is recognized that additional variations of the present invention may be devised without departing from the inventive concept.

What is claimed is:

1. A measuring tool for guiding a cutting member or guide tool to create a portal incision in a hip arthroplasty in communication with a primary incision providing access to an acetabulum, the measuring tool comprising:

a generally L-shaped body comprising

a first elongated body, comprising: a first end, a second end opposite the first end, the first elongated body defining a first axis through the first and second ends of the first elongated body, the second end of the first elongated body having a slot therethrough, the slot defining a slot axis forming an approximately 45 degree angle with the first axis, the slot configured for use in receiving said cutting member or guide tool therethrough and for guiding location of said cutting member or guide tool to create said portal incision relative to said primary incision; and

a second elongated body, comprising: a first end, and a second end opposite the first end, the second elongated body defining a second axis through the first and second ends of the second elongated body, wherein the second end of the second elongated body is connected to the first end of the first body so that the first and second elongated bodies form a generally right angle; and

wherein at least one of the first elongated body or the second elongated body has a plurality of markings evenly spaced apart on its respective body along its respective axis; and

wherein the first end of the first elongated body is adjustable relative to the first end of the second elongated body along the second axis.

2. The measuring tool of claim 1, wherein the second elongated body is telescopic.

3. The measuring tool of claim 1, wherein the slot is mounted on a disc that is connected to the second end of the first elongated slot, the disc being rotatable so as to adjust the slot axis relative to the first axis.

4. The measuring tool of claim 3, wherein the disc comprises markings to identify the angle between the slot axis and the first axis.

5. The measuring tool of claim 4, wherein the disc is configured to rotate automatically when the first elongated member is lengthened or shortened.

6. A measuring tool for guiding a cutting member or guide tool to create a portal incision in a hip arthroplasty in communication with a primary incision providing access to an acetabulum, the measuring tool comprising:

a generally L-shaped body comprising

a first elongated body, comprising: a first end, a second end opposite the first end, the first elongated body defining a first axis through the first and second ends of the first elongated body, the second end of the first elongated body having a slot therethrough, the slot defining a slot axis forming an approximately 45 degree angle with the first axis, the slot configured for use in receiving said cutting member or guide tool therethrough and for guiding location of said cutting member or guide tool to create said portal incision relative to said primary incision; and

26

a second elongated body, comprising: a first end, and a second end opposite the first end, the second elongated body defining a second axis through the first and second ends of the second elongated body, wherein the second end of the second elongated body is connected to the first end of the first body so that the first and second elongated bodies form a generally right angle; and

wherein the second end of the first elongated body is adjustable relative to the second axis and along the first axis.

7. The measuring tool of claim 6, wherein the first elongated body is telescopic.

8. A measuring tool for guiding a cutting member or guide tool to create a portal incision in a hip arthroplasty in communication with a primary incision providing access to an acetabulum, the measuring tool comprising:

a generally L-shaped body comprising

a first elongated body, comprising: a first end, a second end opposite the first end, the first elongated body defining a first axis through the first and second ends of the first elongated body, the second end of the first elongated body having a slot therethrough, the slot defining a slot axis capable of forming an approximately 45 degree angle with the first axis, the slot configured for use in receiving said cutting member or guide tool therethrough and for guiding location of said cutting member or guide tool to create said portal incision relative to said primary incision; and

a second elongated body sized and configured for insertion through said primary incision to said acetabulum, comprising: a first end, and a second end opposite the first end, the second elongated body defining a second axis through the first and second ends of the second elongated body, wherein the second end of the second elongated body is connected to the first end of the first body so that the first and second elongated bodies form a generally right angle; and

a hinge connecting the first elongated body to the second elongated body in an adjustable manner, wherein at least one of the first elongated body or the second elongated body has a plurality of markings evenly spaced apart on its respective body along its respective axis, wherein the second end of the first elongated body is adjustable relative to the second end of the second elongated body along the first axis, and wherein the first end of the first elongated body is adjustable relative to the first end of the second elongated body along the second axis.

9. The measuring tool of claim 8, wherein the slot is mounted on a disc that is connected to the second end of the first elongated slot, the disc being rotatable so as to adjust the slot axis relative to the first axis.

10. A measuring tool for guiding a cutting member or guide tool to create a portal incision in a hip arthroplasty in communication with a primary incision providing access to an acetabulum, the measuring tool comprising:

a generally L-shaped body comprising

a first elongated body having a first end and a second end opposite the first end, the first elongated body defining a first axis through the first and second ends of the first elongated body;

a plurality of markings evenly spaced apart on the first elongated body along the first axis; and

a second end of the first elongated body having a slot therethrough, the slot defining a slot axis capable of



forming an approximately 45 degree angle with the first axis, the slot configured for use in receiving said cutting member or guide tool therethrough and for guiding location of said cutting member or guide tool to create said portal incision relative to said primary incision; and

- a second elongated body sized and configured for insertion through said primary incision to said acetabulum, the second elongated body having a first end and a second end opposite the first end, the second elongated body defining a second axis through the first and second ends of the second elongated body, wherein the second elongated body comprises a plurality of markings evenly spaced apart on the second elongated body along the second axis, wherein the second end of the second elongated body is connected to the first end of the first elongated body so that the first and second elongated bodies form a generally right angle.

**11.** The measuring tool of claim **10**, wherein the slot is mounted on a disc that is connected to the second end of the first elongated slot, the disc being rotatable so as to adjust the slot axis relative to the first axis.

**12.** The measuring tool of claim **11**, wherein the disc comprises markings to identify the angle between the slot axis and the first axis.

**13.** The measuring tool of claim **10**, wherein the first elongated body is telescopic.

**14.** The measuring tool of claim **10**, wherein the second elongated body is telescopic.

**15.** The measuring tool of claim **10**, wherein the first elongated body is telescopic.

\* \* \* \* \*