



US010835250B2

(12) **United States Patent**  
**Weisenburgh, II et al.**

(10) **Patent No.:** **US 10,835,250 B2**  
(45) **Date of Patent:** **Nov. 17, 2020**

(54) **END EFFECTOR COUPLING  
ARRANGEMENTS FOR A SURGICAL  
CUTTING AND STAPLING INSTRUMENT**

(71) Applicant: **Ethicon LLC**, Guaynabo, PR (US)

(72) Inventors: **William B. Weisenburgh, II**,  
Maineville, OH (US); **Jerome R.  
Morgan**, Cincinnati, OH (US); **Kyle P.  
Moore**, Woodstock, GA (US); **Mark H.  
Ransick**, West Chester, OH (US);  
**Steven G. Hall**, Cincinnati, OH (US);  
**Randall J. Tanguay**, Lebanon, OH  
(US); **Jeffrey D. Messerly**, Cincinnati,  
OH (US); **Galen C. Robertson**, Apex,  
NC (US); **Andrew M. Zwolinski**,  
Cincinnati, OH (US); **Jeffrey S.  
Swayze**, West Chester, OH (US);  
**Thomas W. Huitema**, Cincinnati, OH  
(US); **Glen A. Armstrong**, Hamilton,  
OH (US); **Shailendra K Parihar**,  
Mason, OH (US); **Donna L. Korvick**,  
Bridgewater, NJ (US); **Richard W.  
Timm**, Cincinnati, OH (US); **Kevin R.  
Doll**, Mason, OH (US); **Bret W. Smith**,  
South Lebanon, OH (US); **William D.  
Kelly**, Mason, OH (US); **Ronald J.  
Kolata**, Raleigh, NC (US); **Joshua R.  
Uth**, Mason, OH (US); **Charles J.  
Scheib**, Loveland, OH (US); **Geoffrey  
C. Hueil**, Cincinnati, OH (US); **Mark  
S. Ortiz**, Milford, OH (US); **Douglas  
B. Hoffman**, Harrison, OH (US);  
**Patrick A. Weizman**, Liberty  
Township, OH (US); **Dean B. Bruewer**,  
Fairfield, OH (US); **Gregory B. Blair**,  
McCordsville, IN (US); **Frederick E.  
Shelton, IV**, Hillsboro, OH (US)

(73) Assignee: **Ethicon LLC**, Guaynabo, PR (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 171 days.

(21) Appl. No.: **15/793,527**

(22) Filed: **Oct. 25, 2017**

(65) **Prior Publication Data**  
US 2018/0103954 A1 Apr. 19, 2018

**Related U.S. Application Data**

(63) Continuation of application No. 14/672,620, filed on Mar. 30, 2015, now Pat. No. 9,913,647, which is a (Continued)

(51) **Int. Cl.**  
*A61B 17/068* (2006.01)  
*A61B 17/072* (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... *A61B 17/105* (2013.01); *A61B 17/068* (2013.01); *A61B 17/07207* (2013.01);  
(Continued)

(58) **Field of Classification Search**  
CPC ..... A61B 17/05; A61B 17/068; A61B 2017/2931  
(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

2,853,074 A 9/1958 Olson  
3,079,606 A 3/1963 Bobrov et al.  
(Continued)

**FOREIGN PATENT DOCUMENTS**

AU 2012200178 B2 7/2013  
CN 1163558 A 10/1997  
(Continued)



**OTHER PUBLICATIONS**

Serial Communication Protocol; Michael Lemmon Feb. 1, 2009; <http://www3.nd.edu/~lemmon/courses/ee224/web-manual/web-manual/lab12/node2.html>; Wayback Machine to Apr. 29, 2012.  
(Continued)

*Primary Examiner* — Michelle Lopez

(57) **ABSTRACT**

A surgical stapling assembly comprising a firing member, an end effector, a closure member, and a shaft including an attachment interface is disclosed. The surgical stapling assembly is configured to be attached to a surgical instrument interface by way of the attachment interface. The end effector comprises a first jaw, a second jaw, and a staple cartridge comprising staples configured to be ejected by the firing member. The second jaw is movable relative to the  
(Continued)

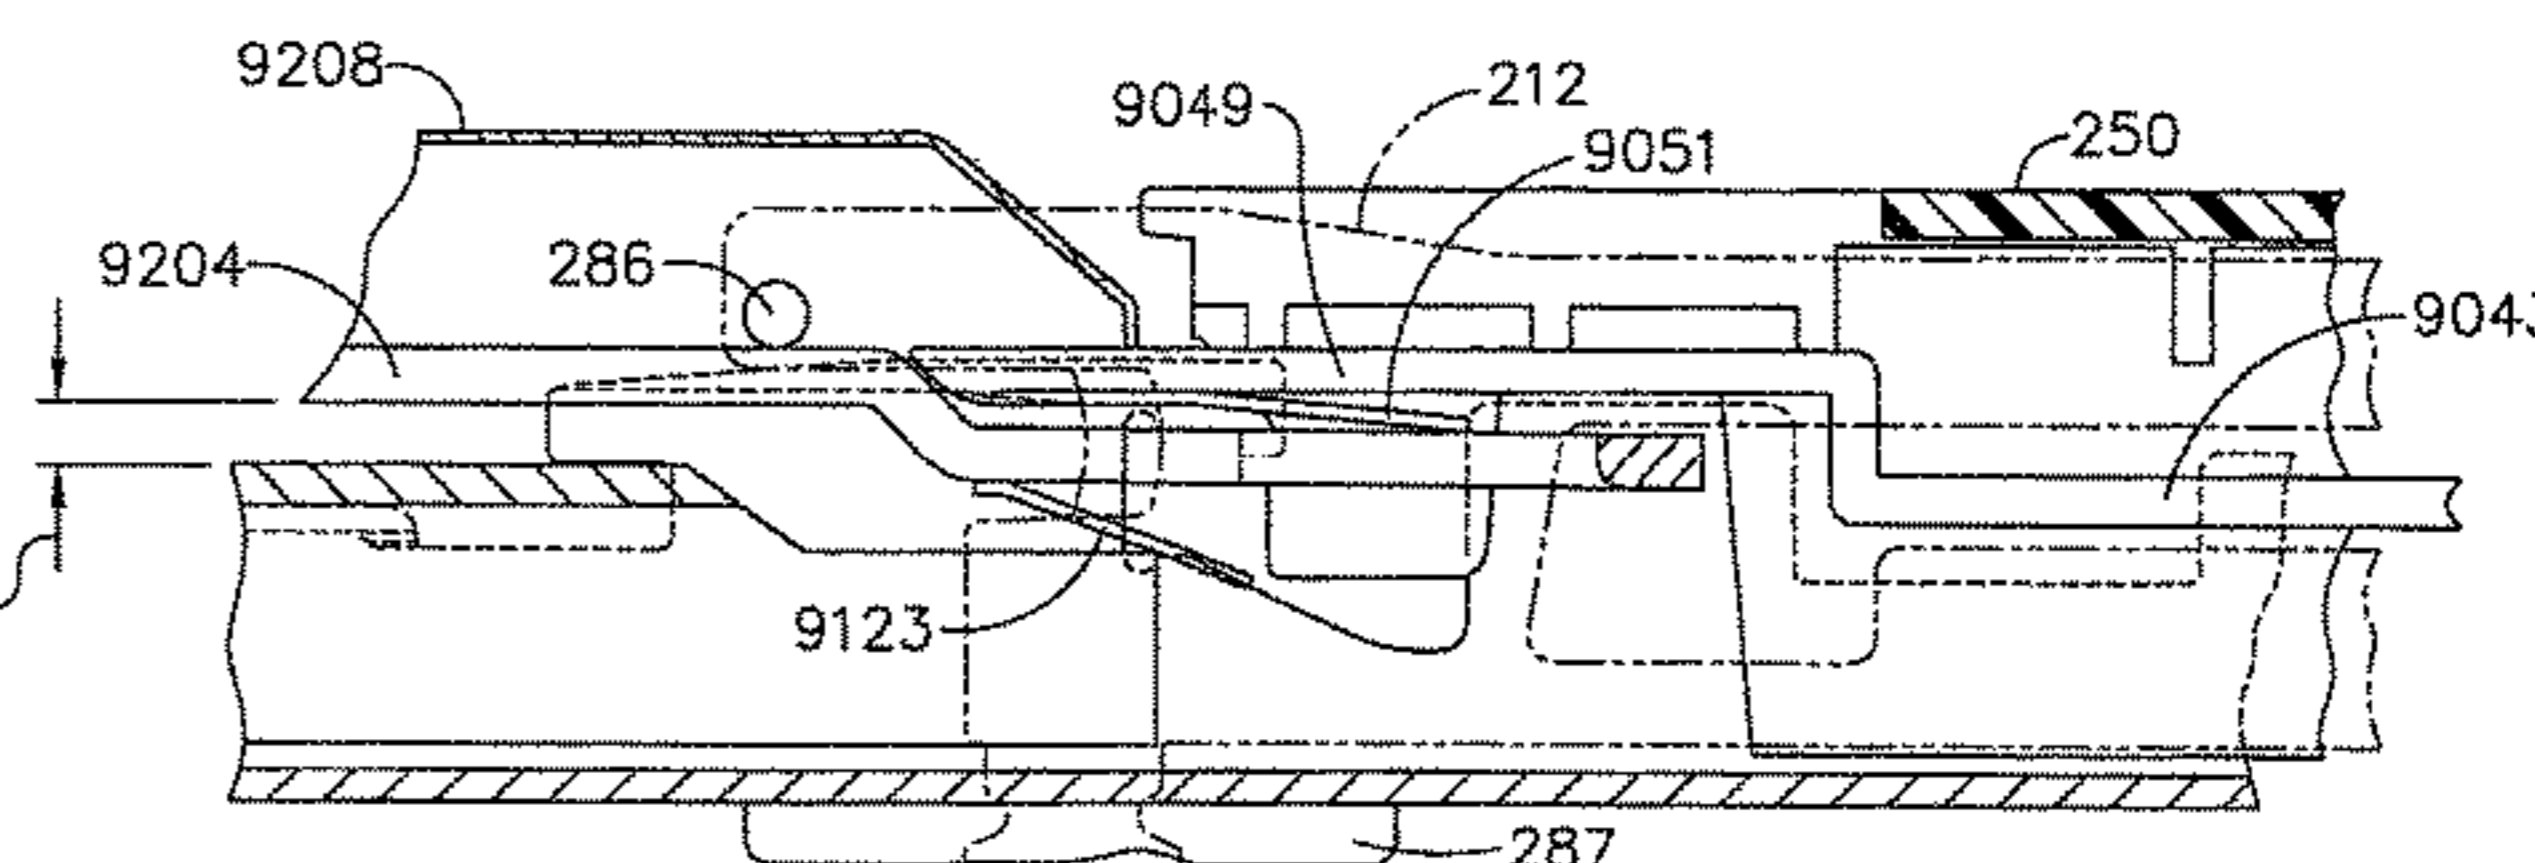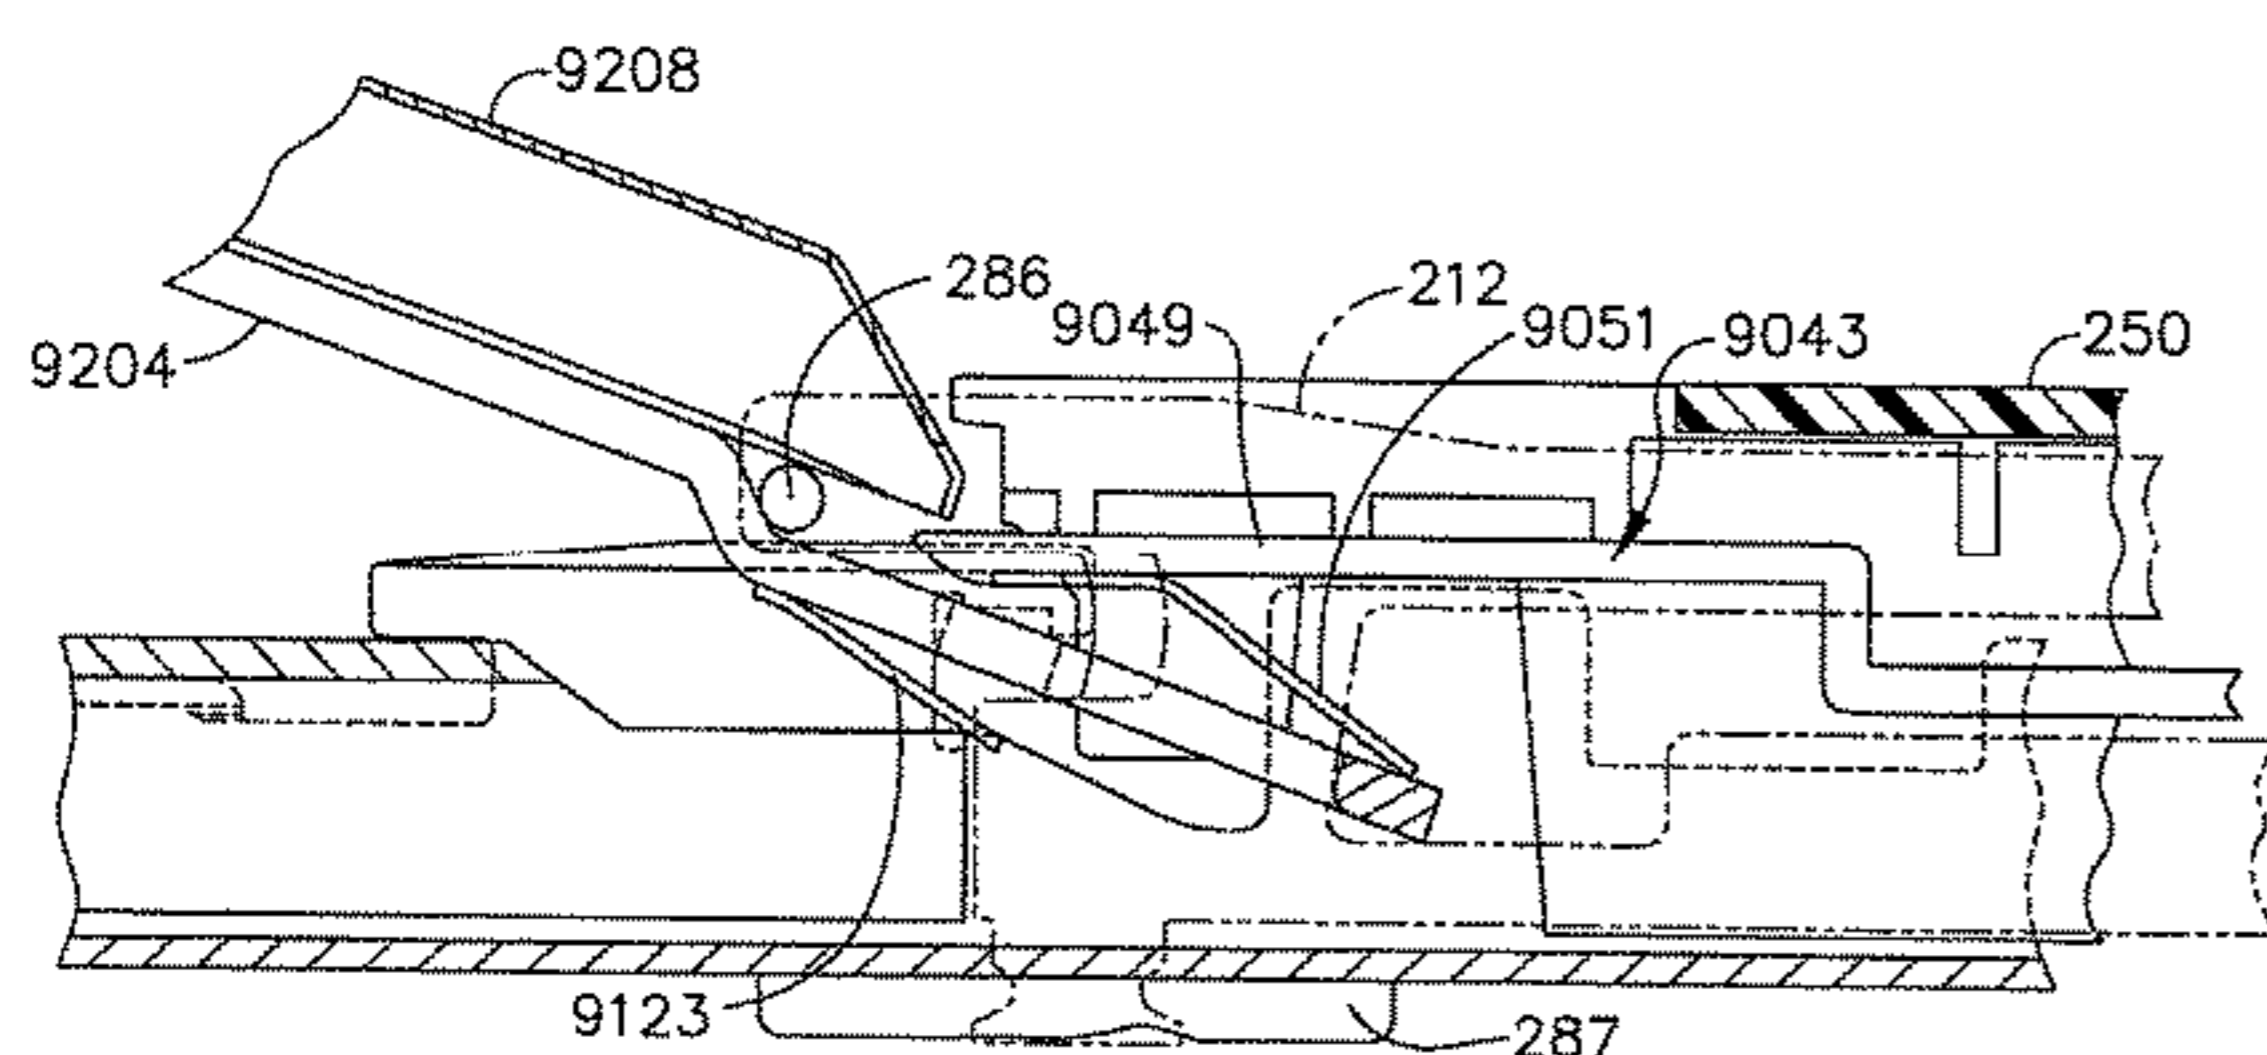

first jaw between an open position, a fully-clamped position, and a collapsed position. The end effector further comprises an interconnection between the first jaw and the second jaw defining a rotational axis about which the second jaw is movable relative to the first jaw. The rotational axis is shiftable toward and away from the first jaw as the second jaw is moved between the open position, the fully-clamped position, and the collapsed position.

**9 Claims, 88 Drawing Sheets**

**Related U.S. Application Data**

continuation of application No. 14/528,626, filed on Oct. 30, 2014, now abandoned, which is a continuation of application No. 13/027,641, filed on Feb. 15, 2011, now Pat. No. 8,875,972, which is a continuation of application No. 12/031,817, filed on Feb. 15, 2008, now abandoned.

(51) **Int. Cl.**

*A61B 17/10* (2006.01)  
*A61B 17/3209* (2006.01)  
*A61B 17/3205* (2006.01)  
*A61B 17/00* (2006.01)  
*A61B 17/29* (2006.01)

(52) **U.S. Cl.**

CPC ..... *A61B 17/3205* (2013.01); *A61B 17/3209* (2013.01); *A61B 2017/00473* (2013.01); *A61B 2017/07214* (2013.01); *A61B 2017/2931* (2013.01)

(58) **Field of Classification Search**

USPC ..... 227/175.1, 175.4  
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,490,675 A 1/1970 Green et al.  
 3,494,533 A 2/1970 Green et al.  
 3,499,591 A 3/1970 Green  
 3,551,987 A 1/1971 Wilkinson  
 3,643,851 A 2/1972 Green et al.  
 3,662,939 A 5/1972 Bryan  
 3,717,294 A 2/1973 Green  
 3,819,100 A 6/1974 Noiles et al.  
 3,952,747 A 4/1976 Kimmell, Jr.  
 RE28,932 E 8/1976 Noiles et al.  
 4,111,206 A 9/1978 Vishnevsky et al.  
 4,127,227 A 11/1978 Green  
 4,135,517 A 1/1979 Reale  
 4,198,982 A 4/1980 Fortner et al.  
 4,207,898 A 6/1980 Becht  
 4,272,002 A 6/1981 Moshofsky  
 4,305,539 A 12/1981 Korolkov et al.  
 4,331,277 A 5/1982 Green  
 4,379,457 A 4/1983 Gravener et al.  
 4,383,634 A 5/1983 Green  
 4,396,139 A 8/1983 Hall et al.  
 4,397,311 A 8/1983 Kanshin et al.  
 4,402,445 A 9/1983 Green  
 4,415,112 A 11/1983 Green  
 4,429,695 A 2/1984 Green  
 4,434,796 A 3/1984 Karapetian et al.  
 4,438,659 A 3/1984 Desplats  
 4,475,679 A 10/1984 Fleury, Jr.  
 4,489,875 A 12/1984 Crawford et al.  
 4,500,024 A 2/1985 DiGiovanni et al.  
 4,505,272 A 3/1985 Utyamyshev et al.

4,505,414 A 3/1985 Filipi  
 4,506,671 A 3/1985 Green  
 4,520,817 A 6/1985 Green  
 4,522,327 A 6/1985 Korthoff et al.  
 4,530,453 A 7/1985 Green  
 4,566,620 A 1/1986 Green et al.  
 4,569,469 A 2/1986 Mongeon et al.  
 4,573,468 A 3/1986 Conta et al.  
 4,573,622 A 3/1986 Green et al.  
 4,576,167 A 3/1986 Noiles  
 4,580,712 A 4/1986 Green  
 4,585,153 A 4/1986 Failla et al.  
 4,605,001 A 8/1986 Rothfuss et al.  
 4,605,004 A 8/1986 Di Giovanni et al.  
 4,608,981 A 9/1986 Rothfuss et al.  
 4,610,383 A 9/1986 Rothfuss et al.  
 4,612,933 A 9/1986 Brinkerhoff et al.  
 4,619,262 A 10/1986 Taylor  
 4,619,391 A 10/1986 Sharkany et al.  
 4,629,107 A 12/1986 Fedotov et al.  
 4,632,290 A 12/1986 Green et al.  
 4,633,874 A 1/1987 Chow et al.  
 4,634,419 A 1/1987 Kreizman et al.  
 4,652,820 A 3/1987 Maresca  
 4,662,555 A 5/1987 Thornton  
 4,664,305 A 5/1987 Blake, III et al.  
 4,665,916 A 5/1987 Green  
 4,669,647 A 6/1987 Storace  
 4,671,445 A 6/1987 Barker et al.  
 4,684,051 A 8/1987 Akopov et al.  
 4,700,703 A 10/1987 Resnick et al.  
 4,708,141 A 11/1987 Inoue et al.  
 4,715,520 A 12/1987 Roehr, Jr. et al.  
 4,719,917 A 1/1988 Barrows et al.  
 4,727,308 A 2/1988 Huljak et al.  
 4,728,020 A 3/1988 Green et al.  
 4,747,820 A 5/1988 Hornlein et al.  
 4,750,902 A 6/1988 Wuchinich et al.  
 4,752,024 A 6/1988 Green et al.  
 4,754,909 A 7/1988 Barker et al.  
 4,767,044 A 8/1988 Green  
 4,773,420 A 9/1988 Green  
 4,805,823 A 2/1989 Rothfuss  
 4,809,695 A 3/1989 Gwathmey et al.  
 4,817,847 A 4/1989 Redtenbacher et al.  
 4,819,853 A 4/1989 Green  
 4,821,939 A 4/1989 Green  
 4,827,911 A 5/1989 Broadwin et al.  
 4,844,068 A 7/1989 Arata et al.  
 4,848,637 A 7/1989 Pruitt  
 4,865,030 A 9/1989 Polyak  
 4,869,414 A 9/1989 Green et al.  
 4,869,415 A 9/1989 Fox  
 4,873,977 A 10/1989 Avant et al.  
 4,893,622 A 1/1990 Green et al.  
 4,896,678 A 1/1990 Ogawa  
 4,903,697 A 2/1990 Resnick et al.  
 4,919,679 A 4/1990 Averill et al.  
 4,930,674 A 6/1990 Barak  
 4,931,047 A 6/1990 Broadwin et al.  
 4,938,408 A 7/1990 Bedi et al.  
 4,941,623 A 7/1990 Pruitt  
 4,944,443 A 7/1990 Oddsen et al.  
 4,978,049 A 12/1990 Green  
 4,978,333 A 12/1990 Broadwin et al.  
 4,986,808 A 1/1991 Broadwin et al.  
 5,002,553 A 3/1991 Shiber  
 5,015,227 A 5/1991 Broadwin et al.  
 5,038,109 A 8/1991 Goble et al.  
 5,040,715 A 8/1991 Green et al.  
 5,065,929 A 11/1991 Schulze et al.  
 5,074,454 A 12/1991 Peters  
 5,088,997 A 2/1992 Delahuerga et al.  
 5,104,397 A 4/1992 Vasconcelos et al.  
 5,125,876 A 6/1992 Hirota  
 5,129,570 A 7/1992 Schulze et al.  
 5,137,198 A 8/1992 Nobis et al.  
 5,139,513 A 8/1992 Segato  
 5,141,144 A 8/1992 Foslien et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,156,315 A	10/1992	Green et al.	5,503,638 A	4/1996	Cooper et al.
5,156,614 A	10/1992	Green et al.	5,505,363 A	4/1996	Green et al.
5,170,925 A	12/1992	Madden et al.	5,507,426 A	4/1996	Young et al.
5,190,517 A	3/1993	Zieve et al.	5,509,596 A	4/1996	Green et al.
5,197,649 A	3/1993	Bessler et al.	5,509,916 A	4/1996	Taylor
5,221,036 A	6/1993	Takase	5,520,678 A	5/1996	Heckele et al.
5,221,281 A	6/1993	Kliccek	5,529,235 A	6/1996	Boiarski et al.
5,240,163 A	8/1993	Stein et al.	5,533,661 A	7/1996	Main et al.
5,258,012 A	11/1993	Luscombe et al.	5,535,934 A	7/1996	Boiarski et al.
5,263,629 A	11/1993	Trumbull et al.	5,535,935 A	7/1996	Vidal et al.
5,281,216 A	1/1994	Kliccek	5,535,937 A	7/1996	Boiarski et al.
5,284,128 A	2/1994	Hart	5,540,375 A	7/1996	Bolanos et al.
5,289,963 A	3/1994	McGarry et al.	5,541,376 A	7/1996	Ladtkow et al.
5,307,976 A	5/1994	Olson et al.	5,542,594 A	8/1996	McKean et al.
5,308,576 A	5/1994	Green et al.	5,547,117 A	8/1996	Hamblin et al.
5,312,023 A	5/1994	Green et al.	5,549,637 A	8/1996	Crainich
5,312,329 A	5/1994	Beaty et al.	5,551,622 A	9/1996	Yoon
5,318,221 A	6/1994	Green et al.	5,553,765 A	9/1996	Knodel et al.
5,326,013 A	7/1994	Green et al.	5,560,530 A	10/1996	Bolanos et al.
5,332,142 A	7/1994	Robinson et al.	5,560,532 A	10/1996	DeFonzo et al.
5,333,772 A	8/1994	Rothfuss et al.	5,562,239 A	10/1996	Boiarski et al.
5,333,773 A	8/1994	Main et al.	5,562,241 A	10/1996	Knodel et al.
5,346,504 A	9/1994	Ortiz et al.	5,564,615 A	10/1996	Bishop et al.
5,358,506 A	10/1994	Green et al.	5,573,541 A	11/1996	Green et al.
5,364,001 A	11/1994	Bryan	5,577,654 A	11/1996	Bishop
5,366,134 A	11/1994	Green et al.	5,579,978 A	12/1996	Green et al.
5,370,645 A	12/1994	Kliccek et al.	5,580,067 A	12/1996	Hamblin et al.
5,372,596 A	12/1994	Kliccek et al.	5,584,425 A	12/1996	Savage et al.
5,374,277 A	12/1994	Hassler	5,586,711 A	12/1996	Plyley et al.
5,382,247 A	1/1995	Cimino et al.	5,588,579 A	12/1996	Schnut et al.
5,383,880 A	1/1995	Hooven	5,588,580 A	12/1996	Paul et al.
5,389,104 A	2/1995	Hahnen et al.	5,588,581 A	12/1996	Conlon et al.
5,395,033 A	3/1995	Byrne et al.	5,597,107 A	1/1997	Knodel et al.
5,395,384 A	3/1995	Duthoit et al.	5,599,344 A	2/1997	Paterson
5,403,312 A	4/1995	Yates et al.	5,601,224 A	2/1997	Bishop et al.
5,405,072 A	4/1995	Zlock et al.	5,603,443 A	2/1997	Clark et al.
5,405,344 A	4/1995	Williamson et al.	5,605,272 A	2/1997	Witt et al.
5,413,272 A	5/1995	Green et al.	5,605,273 A	2/1997	Hamblin et al.
5,413,573 A	5/1995	Koivukangas	5,607,094 A	3/1997	Clark et al.
5,415,334 A	5/1995	Williamson et al.	5,607,095 A	3/1997	Smith et al.
5,417,361 A	5/1995	Williamson, IV	5,609,285 A	3/1997	Grant et al.
5,421,829 A	6/1995	Olichney et al.	5,609,601 A	3/1997	Kolesa et al.
5,422,567 A	6/1995	Matsunaga	5,611,709 A	3/1997	McAnulty
5,423,471 A	6/1995	Mastri et al.	5,613,966 A	3/1997	Makower et al.
5,423,809 A	6/1995	Kliccek	5,615,820 A	4/1997	Viola
5,431,668 A	7/1995	Burbank, III et al.	5,618,303 A	4/1997	Marlow et al.
5,433,721 A	7/1995	Hooven et al.	5,619,992 A	4/1997	Guthrie et al.
5,438,302 A	8/1995	Goble	5,628,446 A	5/1997	Geiste et al.
5,441,483 A	8/1995	Avitall	5,628,743 A	5/1997	Cimino
5,447,265 A	9/1995	Vidal et al.	5,628,745 A	5/1997	Bek
5,447,417 A	9/1995	Kuhl et al.	5,630,539 A	5/1997	Plyley et al.
5,449,355 A	9/1995	Rhum et al.	5,630,540 A	5/1997	Blewett
5,452,837 A	9/1995	Williamson, IV et al.	5,630,541 A	5/1997	Williamson, IV et al.
5,462,215 A	10/1995	Viola et al.	5,632,432 A	5/1997	Schulze et al.
5,465,819 A	11/1995	Weilant et al.	5,632,433 A	5/1997	Grant et al.
5,465,896 A	11/1995	Allen et al.	5,634,584 A	6/1997	Okorochoa et al.
5,466,020 A	11/1995	Page et al.	5,636,779 A	6/1997	Palmer
5,467,911 A	11/1995	Tsuruta et al.	5,636,780 A	6/1997	Green et al.
5,472,442 A	12/1995	Kliccek	5,639,008 A	6/1997	Gallagher et al.
5,474,057 A	12/1995	Makower et al.	5,645,209 A	7/1997	Green et al.
5,474,223 A	12/1995	Viola et al.	5,647,526 A	7/1997	Green et al.
5,474,566 A	12/1995	Alesi et al.	5,647,869 A	7/1997	Goble et al.
5,480,089 A	1/1996	Blewett	5,651,491 A	7/1997	Heaton et al.
5,482,197 A	1/1996	Green et al.	5,653,373 A	8/1997	Green et al.
5,484,095 A	1/1996	Green et al.	5,653,374 A	8/1997	Young et al.
5,484,398 A	1/1996	Stoddard	5,655,698 A	8/1997	Yoon
5,485,947 A	1/1996	Olson et al.	5,657,921 A	8/1997	Young et al.
5,485,952 A	1/1996	Fontayne	5,662,258 A	9/1997	Knodel et al.
5,487,499 A	1/1996	Sorrentino et al.	5,662,260 A	9/1997	Yoon
5,487,500 A	1/1996	Knodel et al.	5,669,544 A	9/1997	Schulze et al.
5,489,058 A	2/1996	Plyley et al.	5,669,904 A	9/1997	Platt, Jr. et al.
5,496,312 A	3/1996	Kliccek	5,669,907 A	9/1997	Platt, Jr. et al.
5,496,317 A	3/1996	Goble et al.	5,673,840 A	10/1997	Schulze et al.
5,497,933 A	3/1996	DeFonzo et al.	5,673,841 A	10/1997	Schulze et al.
5,503,320 A	4/1996	Webster et al.	5,673,842 A	10/1997	Bittner et al.
			5,678,748 A	10/1997	Plyley et al.
			5,680,981 A	10/1997	Mililli et al.
			5,680,982 A	10/1997	Schulze et al.
			5,680,983 A	10/1997	Plyley et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,685,474 A	11/1997	Seeber	5,902,312 A	5/1999	Frater et al.
5,690,269 A	11/1997	Bolanos et al.	5,908,402 A	6/1999	Blythe
5,692,668 A	12/1997	Schulze et al.	5,911,353 A	6/1999	Bolanos et al.
5,693,020 A	12/1997	Rauh	5,915,616 A	6/1999	Viola et al.
5,693,051 A	12/1997	Schulze et al.	5,918,791 A	7/1999	Sorrentino et al.
5,695,494 A	12/1997	Becker	5,919,198 A	7/1999	Graves, Jr. et al.
5,695,504 A	12/1997	Gifford, III et al.	5,937,951 A	8/1999	Izuchukwu et al.
5,697,542 A	12/1997	Knodel et al.	5,941,442 A	8/1999	Geiste et al.
5,697,543 A	12/1997	Burdorff	5,944,715 A	8/1999	Goble et al.
5,702,387 A	12/1997	Arts et al.	5,947,984 A	9/1999	Whipple
5,704,534 A	1/1998	Huitema et al.	5,947,996 A	9/1999	Logeman
5,706,997 A	1/1998	Green et al.	5,951,552 A	9/1999	Long et al.
5,706,998 A	1/1998	Plyley et al.	5,954,259 A	9/1999	Viola et al.
5,707,392 A	1/1998	Kortenbach	5,964,394 A	10/1999	Robertson
5,709,334 A	1/1998	Sorrentino et al.	5,988,479 A	11/1999	Palmer
5,709,680 A	1/1998	Yates et al.	6,004,319 A	12/1999	Goble et al.
5,711,472 A	1/1998	Bryan	6,010,054 A	1/2000	Johnson et al.
5,713,505 A	2/1998	Huitema	6,012,494 A	1/2000	Balazs
5,713,895 A	2/1998	Lontine et al.	6,013,076 A	1/2000	Goble et al.
5,715,604 A	2/1998	Lanzoni	6,015,406 A	1/2000	Goble et al.
5,715,987 A	2/1998	Kelley et al.	6,027,501 A	2/2000	Goble et al.
5,715,988 A	2/1998	Palmer	6,032,849 A	3/2000	Mastri et al.
5,718,359 A	2/1998	Palmer et al.	6,033,399 A	3/2000	Gines
5,718,360 A	2/1998	Green et al.	6,039,734 A	3/2000	Goble
5,720,744 A	2/1998	Eggleston et al.	6,050,172 A	4/2000	Corves et al.
5,732,871 A	3/1998	Clark et al.	6,050,472 A	4/2000	Shibata
5,732,872 A	3/1998	Bolduc et al.	6,050,996 A	4/2000	Schmaltz et al.
5,735,445 A	4/1998	Vidal et al.	6,053,390 A	4/2000	Green et al.
5,735,874 A	4/1998	Measamer et al.	6,068,627 A	5/2000	Orszulak et al.
5,743,456 A	4/1998	Jones et al.	6,074,401 A	6/2000	Gardiner et al.
5,749,893 A	5/1998	Vidal et al.	6,079,606 A	6/2000	Milliman et al.
5,752,644 A	5/1998	Bolanos et al.	6,083,191 A	7/2000	Rose
5,752,965 A	5/1998	Francis et al.	6,093,186 A	7/2000	Goble
5,758,814 A	6/1998	Gallagher et al.	6,099,551 A	8/2000	Gabbay
5,762,255 A	6/1998	Chrisman et al.	6,102,271 A	8/2000	Longo et al.
5,762,256 A	6/1998	Mastri et al.	6,109,500 A	8/2000	Alli et al.
5,772,659 A	6/1998	Becker et al.	6,117,158 A	9/2000	Measamer et al.
5,776,130 A	7/1998	Buyse et al.	6,119,913 A	9/2000	Adams et al.
5,779,130 A	7/1998	Alesi et al.	6,126,058 A	10/2000	Adams et al.
5,779,131 A	7/1998	Knodel et al.	6,131,789 A	10/2000	Schulze et al.
5,779,132 A	7/1998	Knodel et al.	6,131,790 A	10/2000	Piraka
5,782,396 A	7/1998	Mastri et al.	6,149,660 A	11/2000	Laufer et al.
5,782,397 A	7/1998	Koukline	6,153,292 A	11/2000	Bell et al.
5,782,748 A	7/1998	Palmer et al.	6,155,473 A	12/2000	Tompkins et al.
5,785,232 A	7/1998	Vidal et al.	6,156,056 A	12/2000	Kearns et al.
5,794,834 A	8/1998	Hamblin et al.	6,162,208 A	12/2000	Hipps
5,797,536 A	8/1998	Smith et al.	6,179,195 B1	1/2001	Adams et al.
5,797,537 A	8/1998	Oberlin et al.	6,187,003 B1	2/2001	Buyse et al.
5,797,538 A	8/1998	Heaton et al.	6,193,129 B1	2/2001	Bittner et al.
5,799,857 A	9/1998	Robertson et al.	6,202,914 B1	3/2001	Geiste et al.
5,800,379 A	9/1998	Edwards	6,210,403 B1	4/2001	Klicek
5,807,393 A	9/1998	Williamson, IV et al.	6,213,999 B1	4/2001	Platt, Jr. et al.
5,810,855 A	9/1998	Rayburn et al.	6,228,081 B1	5/2001	Goble
5,814,055 A	9/1998	Knodel et al.	6,228,083 B1	5/2001	Lands et al.
5,820,009 A	10/1998	Melling et al.	6,241,139 B1	6/2001	Milliman et al.
5,826,776 A	10/1998	Schulze et al.	6,241,140 B1	6/2001	Adams et al.
5,827,271 A	10/1998	Buyse et al.	6,250,532 B1	6/2001	Green et al.
5,829,662 A	11/1998	Allen et al.	6,261,286 B1	7/2001	Goble et al.
5,830,598 A	11/1998	Patterson	6,264,086 B1	7/2001	McGuckin, Jr.
5,833,695 A	11/1998	Yoon	6,264,087 B1	7/2001	Whitman
5,836,503 A	11/1998	Ehrenfels et al.	6,273,897 B1	8/2001	Dalessandro et al.
5,839,639 A	11/1998	Sauer et al.	6,277,114 B1	8/2001	Bullivant et al.
5,843,021 A	12/1998	Edwards et al.	6,302,311 B1	10/2001	Adams et al.
5,855,311 A	1/1999	Hamblin et al.	6,315,184 B1	11/2001	Whitman
5,860,581 A	1/1999	Robertson et al.	6,322,494 B1	11/2001	Bullivant et al.
5,860,975 A	1/1999	Goble et al.	6,325,799 B1	12/2001	Goble
5,865,361 A	2/1999	Milliman et al.	6,325,810 B1	12/2001	Hamilton et al.
5,868,790 A	2/1999	Vincent et al.	6,330,965 B1	12/2001	Milliman et al.
5,871,135 A	2/1999	Williamson, IV et al.	6,334,861 B1	1/2002	Chandler et al.
5,878,937 A	3/1999	Green et al.	6,336,926 B1	1/2002	Goble
5,878,938 A	3/1999	Bittner et al.	6,343,731 B1	2/2002	Adams et al.
5,893,506 A	4/1999	Powell	6,358,224 B1	3/2002	Tims et al.
5,894,979 A	4/1999	Powell	H2037 H	7/2002	Yates et al.
5,897,552 A	4/1999	Edwards et al.	6,439,446 B1	8/2002	Perry et al.
5,901,895 A	5/1999	Heaton et al.	6,443,973 B1	9/2002	Whitman
			6,450,391 B1	9/2002	Kayan et al.
			6,478,210 B2	11/2002	Adams et al.
			6,488,196 B1	12/2002	Fenton, Jr.
			6,488,197 B1	12/2002	Whitman

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,491,201 B1	12/2002	Whitman	6,995,729 B2	2/2006	Govari et al.
6,491,690 B1	12/2002	Goble et al.	7,000,818 B2	2/2006	Shelton, IV et al.
6,505,768 B2	1/2003	Whitman	7,000,819 B2	2/2006	Swayze et al.
6,517,528 B1	2/2003	Pantages et al.	7,001,408 B2	2/2006	Knodel et al.
6,517,565 B1	2/2003	Whitman et al.	7,008,435 B2	3/2006	Cummins
6,533,157 B1	3/2003	Whitman	7,018,357 B2	3/2006	Emmons
6,558,379 B1	5/2003	Batchelor et al.	7,023,159 B2	4/2006	Gorti et al.
6,569,085 B2	5/2003	Kortenbach et al.	7,032,798 B2	4/2006	Whitman et al.
6,578,751 B2	6/2003	Hartwick	7,032,799 B2	4/2006	Viola et al.
6,585,144 B2	7/2003	Adams et al.	7,044,352 B2	5/2006	Shelton, IV et al.
6,588,643 B2	7/2003	Bolduc et al.	7,044,353 B2	5/2006	Mastri et al.
6,589,118 B1	7/2003	Soma et al.	7,052,494 B2	5/2006	Goble et al.
6,592,597 B2	7/2003	Grant et al.	7,055,730 B2	6/2006	Ehrenfels et al.
6,601,749 B2	8/2003	Sullivan et al.	7,055,731 B2	6/2006	Shelton, IV et al.
6,607,475 B2	8/2003	Doyle et al.	7,059,508 B2	6/2006	Shelton, IV et al.
6,616,686 B2	9/2003	Coleman et al.	7,070,083 B2	7/2006	Jankowski
6,619,529 B2	9/2003	Green et al.	7,080,769 B2	7/2006	Vresh et al.
6,629,630 B2	10/2003	Adams	7,083,075 B2	8/2006	Swayze et al.
6,629,988 B2	10/2003	Weadock	7,097,089 B2	8/2006	Marczyk
6,644,532 B2	11/2003	Green et al.	7,097,644 B2	8/2006	Long
6,656,193 B2	12/2003	Grant et al.	7,111,769 B2	9/2006	Wales et al.
6,669,073 B2	12/2003	Milliman et al.	7,114,642 B2	10/2006	Whitman
6,670,806 B2	12/2003	Wendt et al.	7,119,534 B2	10/2006	Butzmann
6,676,660 B2	1/2004	Wampler et al.	7,121,446 B2	10/2006	Arad et al.
6,681,978 B2	1/2004	Geiste et al.	7,122,028 B2	10/2006	Looper et al.
6,681,979 B2	1/2004	Whitman	7,128,253 B2	10/2006	Mastri et al.
6,695,198 B2	2/2004	Adams et al.	7,128,254 B2	10/2006	Shelton, IV et al.
6,695,199 B2	2/2004	Whitman	7,128,748 B2	10/2006	Mooradian et al.
6,698,643 B2	3/2004	Whitman	7,133,601 B2	11/2006	Phillips et al.
6,722,552 B2	4/2004	Fenton, Jr.	7,134,587 B2	11/2006	Schwemberger et al.
6,723,109 B2	4/2004	Solingen	7,137,981 B2	11/2006	Long
6,726,697 B2	4/2004	Nicholas et al.	7,140,527 B2	11/2006	Ehrenfels et al.
6,749,560 B1	6/2004	Konstorum et al.	7,140,528 B2	11/2006	Shelton, IV
6,755,338 B2	6/2004	Hahnen et al.	7,143,923 B2	12/2006	Shelton, IV et al.
6,761,685 B2	7/2004	Adams et al.	7,143,924 B2	12/2006	Scirica et al.
6,769,590 B2	8/2004	Vresh et al.	7,143,925 B2	12/2006	Shelton, IV et al.
6,769,594 B2	8/2004	Orban, III	7,143,926 B2	12/2006	Shelton, IV et al.
6,773,437 B2	8/2004	Ogilvie et al.	7,147,138 B2	12/2006	Shelton, IV
6,786,382 B1	9/2004	Hoffman	7,147,139 B2	12/2006	Schwemberger et al.
6,793,652 B1	9/2004	Whitman et al.	7,147,140 B2	12/2006	Wukusick et al.
6,793,661 B2	9/2004	Hamilton et al.	7,147,637 B2	12/2006	Goble
6,805,273 B2	10/2004	Bilotti et al.	7,147,650 B2	12/2006	Lee
6,817,508 B1	11/2004	Racenet et al.	7,150,748 B2	12/2006	Ebbutt et al.
6,817,509 B2	11/2004	Geiste et al.	7,156,824 B2	1/2007	Rosenman
6,817,974 B2	11/2004	Cooper et al.	7,159,750 B2	1/2007	Racenet et al.
6,820,791 B2	11/2004	Adams	7,168,604 B2	1/2007	Milliman et al.
6,827,246 B2	12/2004	Sullivan et al.	7,172,104 B2	2/2007	Scirica et al.
6,830,174 B2	12/2004	Hillstead et al.	7,179,267 B2	2/2007	Nolan et al.
6,835,336 B2	12/2004	Watt	7,182,239 B1	2/2007	Myers
6,840,423 B2	1/2005	Adams et al.	7,188,758 B2	3/2007	Viola et al.
6,843,403 B2	1/2005	Whitman	7,199,537 B2	4/2007	Okamura et al.
6,858,005 B2	2/2005	Ohline et al.	7,204,404 B2	4/2007	Nguyen et al.
RE38,708 E	3/2005	Bolanos et al.	7,204,835 B2	4/2007	Latterell et al.
6,866,178 B2	3/2005	Adams et al.	7,207,471 B2	4/2007	Heinrich et al.
6,874,669 B2	4/2005	Adams et al.	7,207,472 B2	4/2007	Wukusick et al.
6,877,647 B2	4/2005	Green et al.	7,210,609 B2	5/2007	Leiboff et al.
6,878,106 B1	4/2005	Herrmann	7,211,081 B2	5/2007	Goble
6,905,057 B2	6/2005	Swayze et al.	7,213,736 B2	5/2007	Wales et al.
6,908,472 B2	6/2005	Wiener et al.	7,220,272 B2	5/2007	Weadock
6,932,810 B2	8/2005	Ryan	7,225,963 B2	6/2007	Scirica
6,945,444 B2	9/2005	Gresham et al.	7,225,964 B2	6/2007	Mastri et al.
6,951,562 B2	10/2005	Zwirnmann	7,234,624 B2	6/2007	Gresham et al.
6,953,138 B1	10/2005	Dworak et al.	7,237,708 B1	7/2007	Guy et al.
6,953,139 B2	10/2005	Milliman et al.	7,238,195 B2	7/2007	Viola
6,958,035 B2	10/2005	Friedman et al.	7,241,289 B2	7/2007	Braun
6,959,851 B2	11/2005	Heinrich	7,246,734 B2	7/2007	Shelton, IV
6,959,852 B2	11/2005	Shelton, IV et al.	7,247,161 B2	7/2007	Johnston et al.
6,964,363 B2	11/2005	Wales et al.	7,258,262 B2	8/2007	Mastri et al.
6,978,921 B2	12/2005	Shelton, IV et al.	7,258,546 B2	8/2007	Beier et al.
6,978,922 B2	12/2005	Bilotti et al.	7,278,562 B2	10/2007	Mastri et al.
6,981,628 B2	1/2006	Wales	7,278,563 B1	10/2007	Green
6,984,231 B2	1/2006	Goble et al.	7,282,048 B2	10/2007	Goble et al.
6,986,451 B1	1/2006	Mastri et al.	7,287,682 B1	10/2007	Ezzat et al.
6,988,649 B2	1/2006	Shelton, IV et al.	7,293,685 B2	11/2007	Ehrenfels et al.
6,988,650 B2	1/2006	Schwemberger et al.	7,296,722 B2	11/2007	Ivanko
			7,296,724 B2	11/2007	Green et al.
			7,300,450 B2	11/2007	Vleugels et al.
			7,303,106 B2	12/2007	Milliman et al.
			7,303,107 B2	12/2007	Milliman et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

7,303,108 B2	12/2007	Shelton, IV	7,513,408 B2	4/2009	Shelton, IV et al.
7,308,998 B2	12/2007	Mastri et al.	7,517,356 B2	4/2009	Heinrich
7,322,994 B2	1/2008	Nicholas et al.	7,546,939 B2	6/2009	Adams et al.
7,326,203 B2	2/2008	Papineau et al.	7,546,940 B2	6/2009	Milliman et al.
7,328,828 B2	2/2008	Ortiz et al.	7,547,312 B2	6/2009	Bauman et al.
7,328,829 B2	2/2008	Arad et al.	7,549,563 B2	6/2009	Mather et al.
7,331,340 B2	2/2008	Barney	7,549,564 B2	6/2009	Boudreaux
7,331,969 B1	2/2008	Inganas et al.	7,549,998 B2	6/2009	Braun
7,334,717 B2	2/2008	Rethy et al.	7,552,854 B2	6/2009	Wixey et al.
7,334,718 B2	2/2008	McAlister et al.	7,556,185 B2	7/2009	Viola
7,336,048 B2	2/2008	Lohr	7,556,186 B2	7/2009	Milliman
RE40,237 E	4/2008	Bilotti et al.	7,559,449 B2	7/2009	Viola
7,354,447 B2	4/2008	Shelton, IV et al.	7,559,450 B2	7/2009	Wales et al.
7,357,287 B2	4/2008	Shelton, IV et al.	7,559,452 B2	7/2009	Wales et al.
7,357,806 B2	4/2008	Rivera et al.	7,565,993 B2	7/2009	Milliman et al.
7,364,060 B2	4/2008	Milliman	7,568,603 B2	8/2009	Shelton, IV et al.
7,364,061 B2	4/2008	Swayze et al.	7,568,604 B2	8/2009	Ehrenfels et al.
7,380,695 B2	6/2008	Doll et al.	7,575,144 B2	8/2009	Ortiz et al.
7,380,696 B2	6/2008	Shelton, IV et al.	7,588,174 B2	9/2009	Holsten et al.
7,396,356 B2	7/2008	Mollenauer	7,588,175 B2	9/2009	Timm et al.
7,398,907 B2	7/2008	Racenet et al.	7,588,176 B2	9/2009	Timm et al.
7,398,908 B2	7/2008	Holsten et al.	7,588,177 B2	9/2009	Racenet
7,401,721 B2	7/2008	Holsten et al.	7,597,229 B2	10/2009	Boudreaux et al.
7,404,508 B2	7/2008	Smith et al.	7,597,230 B2	10/2009	Racenet et al.
7,404,509 B2	7/2008	Ortiz et al.	7,600,663 B2	10/2009	Green
7,404,822 B2	7/2008	Viart et al.	7,604,150 B2	10/2009	Boudreaux
7,407,074 B2	8/2008	Ortiz et al.	7,604,151 B2	10/2009	Hess et al.
7,407,075 B2	8/2008	Holsten et al.	7,607,557 B2	10/2009	Shelton, IV et al.
7,407,076 B2	8/2008	Racenet et al.	7,615,067 B2	11/2009	Lee et al.
7,407,077 B2	8/2008	Ortiz et al.	7,617,961 B2	11/2009	Viola
7,407,078 B2	8/2008	Shelton, IV et al.	7,624,902 B2	12/2009	Marczyk et al.
7,410,086 B2	8/2008	Ortiz et al.	7,624,903 B2	12/2009	Green et al.
7,416,101 B2	8/2008	Shelton, IV et al.	7,625,370 B2	12/2009	Hart et al.
RE40,514 E	9/2008	Mastri et al.	7,631,793 B2	12/2009	Rethy et al.
7,419,080 B2	9/2008	Smith et al.	7,631,794 B2	12/2009	Rethy et al.
7,419,081 B2	9/2008	Ehrenfels et al.	7,635,074 B2	12/2009	Olson et al.
7,419,321 B2	9/2008	Tereschouk	7,637,409 B2	12/2009	Marczyk
7,422,136 B1	9/2008	Marczyk	7,637,410 B2	12/2009	Marczyk
7,422,138 B2	9/2008	Bilotti et al.	7,638,958 B2	12/2009	Philipp et al.
7,422,139 B2	9/2008	Shelton, IV et al.	7,641,091 B2	1/2010	Olson et al.
7,424,965 B2	9/2008	Racenet et al.	7,641,092 B2	1/2010	Kruszynski et al.
7,427,607 B2	9/2008	Suzuki	7,641,093 B2	1/2010	Doll et al.
7,431,188 B1	10/2008	Marczyk	7,641,095 B2	1/2010	Viola
7,431,189 B2	10/2008	Shelton, IV et al.	7,644,848 B2	1/2010	Swayze et al.
7,431,694 B2	10/2008	Stefanchik et al.	7,645,230 B2	1/2010	Mikkaichi et al.
7,431,730 B2	10/2008	Viola	7,651,017 B2	1/2010	Ortiz et al.
7,434,715 B2	10/2008	Shelton, IV et al.	7,654,431 B2	2/2010	Hueil et al.
7,434,717 B2	10/2008	Shelton, IV et al.	7,658,311 B2	2/2010	Boudreaux
7,438,209 B1	10/2008	Hess et al.	7,658,312 B2	2/2010	Vidal et al.
7,438,718 B2	10/2008	Milliman et al.	7,662,161 B2	2/2010	Briganti et al.
7,441,684 B2	10/2008	Shelton, IV et al.	7,665,646 B2	2/2010	Prommersberger
7,441,685 B1	10/2008	Boudreaux	7,665,647 B2	2/2010	Shelton, IV et al.
7,448,525 B2	11/2008	Shelton, IV et al.	7,669,746 B2	3/2010	Shelton, IV
7,451,904 B2	11/2008	Shelton, IV	7,669,747 B2	3/2010	Weisenburgh, II et al.
7,455,208 B2	11/2008	Wales et al.	7,670,334 B2	3/2010	Hueil et al.
7,461,767 B2	12/2008	Viola et al.	7,673,780 B2	3/2010	Shelton, IV et al.
7,464,846 B2	12/2008	Shelton, IV et al.	7,673,781 B2	3/2010	Swayze et al.
7,464,847 B2	12/2008	Viola et al.	7,673,782 B2	3/2010	Hess et al.
7,464,849 B2	12/2008	Shelton, IV et al.	7,673,783 B2	3/2010	Morgan et al.
7,467,740 B2	12/2008	Shelton, IV et al.	7,686,201 B2	3/2010	Csiky
7,472,814 B2	1/2009	Mastri et al.	7,694,865 B2	4/2010	Scirica
7,472,815 B2	1/2009	Shelton, IV et al.	7,695,485 B2	4/2010	Whitman et al.
7,472,816 B2	1/2009	Holsten et al.	7,699,204 B2	4/2010	Viola
7,473,253 B2	1/2009	Dycus et al.	7,699,846 B2	4/2010	Ryan
7,481,347 B2	1/2009	Roy	7,699,856 B2	4/2010	Van Wyk et al.
7,481,348 B2	1/2009	Marczyk	7,703,653 B2	4/2010	Shah et al.
7,481,349 B2	1/2009	Holsten et al.	7,708,180 B2	5/2010	Murray et al.
7,487,899 B2	2/2009	Shelton, IV et al.	7,708,181 B2	5/2010	Cole et al.
7,490,749 B2	2/2009	Schall et al.	7,708,182 B2	5/2010	Viola
7,494,039 B2	2/2009	Racenet et al.	7,708,758 B2	5/2010	Lee et al.
7,500,979 B2	3/2009	Hueil et al.	7,717,312 B2	5/2010	Beetel
7,503,474 B2	3/2009	Hillstead et al.	7,717,313 B2	5/2010	Criscuolo et al.
7,506,790 B2	3/2009	Shelton, IV	7,717,846 B2	5/2010	Zirps et al.
7,506,791 B2	3/2009	Omaits et al.	7,721,930 B2	5/2010	McKenna et al.
7,510,107 B2	3/2009	Timm et al.	7,721,931 B2	5/2010	Shelton, IV et al.
			7,721,933 B2	5/2010	Ehrenfels et al.
			7,721,934 B2	5/2010	Shelton, IV et al.
			7,721,936 B2	5/2010	Shelton, IV et al.
			7,725,214 B2	5/2010	Diolaiti

(56)

## References Cited

## U.S. PATENT DOCUMENTS

7,726,537 B2	6/2010	Olson et al.	7,905,380 B2	3/2011	Shelton, IV et al.
7,726,538 B2	6/2010	Holsten et al.	7,905,381 B2	3/2011	Baxter, III et al.
7,726,539 B2	6/2010	Holsten et al.	7,905,893 B2	3/2011	Kuhns et al.
7,731,072 B2	6/2010	Timm et al.	7,909,039 B2	3/2011	Hur
7,731,073 B2	6/2010	Wixey et al.	7,909,220 B2	3/2011	Viola
7,735,703 B2	6/2010	Morgan et al.	7,909,221 B2	3/2011	Viola et al.
7,738,971 B2	6/2010	Swayze et al.	7,913,891 B2	3/2011	Doll et al.
7,740,159 B2	6/2010	Shelton, IV et al.	7,913,893 B2	3/2011	Mastri et al.
7,743,960 B2	6/2010	Whitman et al.	7,918,230 B2	4/2011	Whitman et al.
7,744,627 B2	6/2010	Orban, III et al.	7,918,376 B1	4/2011	Knodel et al.
7,751,870 B2	7/2010	Whitman	7,918,377 B2	4/2011	Measamer et al.
7,753,245 B2	7/2010	Boudreaux et al.	7,918,845 B2	4/2011	Saadat et al.
7,753,904 B2	7/2010	Shelton, IV et al.	7,922,061 B2	4/2011	Shelton, IV et al.
7,766,209 B2	8/2010	Baxter, III et al.	7,922,063 B2	4/2011	Zemlok et al.
7,766,210 B2	8/2010	Shelton, IV et al.	7,922,743 B2	4/2011	Heinrich et al.
7,770,773 B2	8/2010	Whitman et al.	7,926,691 B2	4/2011	Viola et al.
7,770,774 B2	8/2010	Mastri et al.	7,931,660 B2	4/2011	Aranyi et al.
7,770,775 B2	8/2010	Shelton, IV et al.	7,934,630 B2	5/2011	Shelton, IV et al.
7,770,776 B2	8/2010	Chen et al.	7,934,631 B2	5/2011	Balbierz et al.
7,780,054 B2	8/2010	Wales	7,935,773 B2	5/2011	Hadba et al.
7,780,055 B2	8/2010	Scirica et al.	7,938,307 B2	5/2011	Bettuchi
7,784,662 B2	8/2010	Wales et al.	7,942,303 B2	5/2011	Shah
7,784,663 B2	8/2010	Shelton, IV	7,942,890 B2	5/2011	D'Agostino et al.
7,793,812 B2	9/2010	Moore et al.	7,950,560 B2	5/2011	Zemlok et al.
7,794,475 B2	9/2010	Hess et al.	7,950,561 B2	5/2011	Aranyi
7,798,386 B2	9/2010	Schall et al.	7,951,071 B2	5/2011	Whitman et al.
7,799,039 B2	9/2010	Shelton, IV et al.	7,954,682 B2	6/2011	Giordano et al.
7,803,151 B2	9/2010	Whitman	7,954,684 B2	6/2011	Boudreaux
7,810,690 B2	10/2010	Bilotti et al.	7,954,686 B2	6/2011	Baxter, III et al.
7,810,691 B2	10/2010	Boyden et al.	7,954,687 B2	6/2011	Zemlok et al.
7,810,692 B2	10/2010	Hall et al.	7,959,050 B2	6/2011	Smith et al.
7,810,693 B2	10/2010	Broehl et al.	7,959,051 B2	6/2011	Smith et al.
7,815,092 B2	10/2010	Whitman et al.	7,959,052 B2	6/2011	Sonnenschein et al.
7,819,296 B2	10/2010	Hueil et al.	7,963,432 B2	6/2011	Knodel et al.
7,819,297 B2	10/2010	Doll et al.	7,963,433 B2	6/2011	Whitman et al.
7,819,298 B2	10/2010	Hall et al.	7,966,799 B2	6/2011	Morgan et al.
7,819,299 B2	10/2010	Shelton, IV et al.	7,967,178 B2	6/2011	Scirica et al.
7,823,592 B2	11/2010	Bettuchi et al.	7,967,179 B2	6/2011	Olson et al.
7,823,760 B2	11/2010	Zemlok et al.	7,967,180 B2	6/2011	Scirica
7,828,189 B2	11/2010	Holsten et al.	7,967,181 B2	6/2011	Viola et al.
7,832,408 B2	11/2010	Shelton, IV et al.	7,967,839 B2	6/2011	Flock et al.
7,832,611 B2	11/2010	Boyden et al.	7,972,298 B2	7/2011	Wallace et al.
7,832,612 B2	11/2010	Baxter, III et al.	7,976,563 B2	7/2011	Summerer
7,837,079 B2	11/2010	Holsten et al.	7,980,443 B2	7/2011	Scheib et al.
7,837,080 B2	11/2010	Schwemberger	7,988,026 B2	8/2011	Knodel et al.
7,837,081 B2	11/2010	Holsten et al.	7,988,027 B2	8/2011	Olson et al.
7,837,694 B2	11/2010	Tethrake et al.	7,988,028 B2	8/2011	Farascioni et al.
7,841,503 B2	11/2010	Sonnenschein et al.	7,988,779 B2	8/2011	Disalvo et al.
7,842,028 B2	11/2010	Lee	7,992,757 B2	8/2011	Wheeler et al.
7,845,533 B2	12/2010	Marczyk et al.	7,997,468 B2	8/2011	Farascioni
7,845,534 B2	12/2010	Viola et al.	7,997,469 B2	8/2011	Olson et al.
7,845,535 B2	12/2010	Scircia	8,002,795 B2	8/2011	Beetel
7,845,536 B2	12/2010	Viola et al.	8,006,885 B2	8/2011	Marczyk
7,845,537 B2	12/2010	Shelton, IV et al.	8,006,889 B2	8/2011	Adams et al.
7,854,736 B2	12/2010	Ryan	8,011,550 B2	9/2011	Aranyi et al.
7,857,183 B2	12/2010	Shelton, IV	8,011,551 B2	9/2011	Marczyk et al.
7,857,185 B2	12/2010	Swayze et al.	8,011,553 B2	9/2011	Mastri et al.
7,857,186 B2	12/2010	Baxter, III et al.	8,011,555 B2	9/2011	Tarinelli et al.
7,861,906 B2	1/2011	Doll et al.	8,016,176 B2	9/2011	Kasvikis et al.
7,866,525 B2	1/2011	Scirica	8,016,177 B2	9/2011	Bettuchi et al.
7,866,527 B2	1/2011	Hall et al.	8,016,178 B2	9/2011	Olson et al.
7,866,528 B2	1/2011	Olson et al.	8,016,849 B2	9/2011	Wenchell
7,870,989 B2	1/2011	Viola et al.	8,016,855 B2	9/2011	Whitman et al.
7,886,951 B2	2/2011	Hessler	8,016,858 B2	9/2011	Whitman
7,886,952 B2	2/2011	Scirica et al.	8,020,742 B2	9/2011	Marczyk
7,887,530 B2	2/2011	Zemlok et al.	8,020,743 B2	9/2011	Shelton, IV
7,887,563 B2	2/2011	Cummins	8,021,377 B2	9/2011	Eskuri
7,891,531 B1	2/2011	Ward	8,025,199 B2	9/2011	Whitman et al.
7,891,532 B2	2/2011	Mastri et al.	8,028,883 B2	10/2011	Stopek
7,892,245 B2	2/2011	Liddicoat et al.	8,028,884 B2	10/2011	Sniffin et al.
7,893,586 B2	2/2011	West et al.	8,028,885 B2	10/2011	Smith et al.
7,896,214 B2	3/2011	Farascioni	8,033,438 B2	10/2011	Scirica
7,896,215 B2	3/2011	Adams et al.	8,033,440 B2	10/2011	Wenchell et al.
7,896,877 B2	3/2011	Hall et al.	8,035,487 B2	10/2011	Malackowski
7,900,805 B2	3/2011	Shelton, IV et al.	8,038,045 B2	10/2011	Bettuchi et al.
			8,038,046 B2	10/2011	Smith et al.
			8,047,236 B2	11/2011	Perry
			8,056,787 B2	11/2011	Boudreaux et al.
			8,056,788 B2	11/2011	Mastri et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,061,576 B2	11/2011	Cappola	8,256,654 B2	9/2012	Bettuchi et al.
8,062,330 B2	11/2011	Prommersberger et al.	8,256,655 B2	9/2012	Sniffin et al.
8,066,166 B2	11/2011	Demmy et al.	8,256,656 B2	9/2012	Milliman et al.
8,066,167 B2	11/2011	Measamer et al.	8,267,300 B2	9/2012	Boudreaux
8,066,168 B2	11/2011	Vidal et al.	8,272,553 B2	9/2012	Mastri et al.
D650,074 S	12/2011	Hunt et al.	8,272,554 B2	9/2012	Whitman et al.
8,070,035 B2	12/2011	Holsten et al.	8,276,801 B2	10/2012	Zemlok et al.
8,083,118 B2	12/2011	Milliman et al.	8,276,802 B2	10/2012	Kostrzewski
8,083,119 B2	12/2011	Prommersberger	8,281,973 B2	10/2012	Wenchell et al.
8,083,120 B2	12/2011	Shelton, IV et al.	8,281,974 B2	10/2012	Hessler et al.
8,091,756 B2	1/2012	Viola	8,286,845 B2	10/2012	Perry et al.
8,092,932 B2	1/2012	Phillips et al.	8,286,846 B2	10/2012	Smith et al.
8,096,458 B2	1/2012	Hessler	8,292,150 B2	10/2012	Bryant
8,097,017 B2	1/2012	Viola	8,292,151 B2	10/2012	Viola
8,100,310 B2	1/2012	Zemlok	8,292,155 B2	10/2012	Shelton, IV et al.
8,105,350 B2	1/2012	Lee et al.	8,292,157 B2	10/2012	Smith et al.
8,109,426 B2	2/2012	Milliman et al.	8,292,888 B2	10/2012	Whitman
8,113,405 B2	2/2012	Milliman	8,308,040 B2	11/2012	Huang et al.
8,113,410 B2	2/2012	Hall et al.	8,308,042 B2	11/2012	Aranyi
8,114,100 B2	2/2012	Smith et al.	8,308,043 B2	11/2012	Bindra et al.
8,123,103 B2	2/2012	Milliman	8,308,046 B2	11/2012	Prommersberger
8,127,975 B2	3/2012	Olson et al.	8,313,496 B2	11/2012	Sauer et al.
8,127,976 B2	3/2012	Scirica et al.	8,317,070 B2	11/2012	Hueil et al.
8,132,703 B2	3/2012	Milliman et al.	8,317,071 B1	11/2012	Knodel
8,132,706 B2	3/2012	Marczyk et al.	8,317,074 B2	11/2012	Ortiz et al.
8,136,712 B2	3/2012	Zingman	8,317,744 B2	11/2012	Kirschenman
8,136,713 B2	3/2012	Hathaway et al.	8,322,455 B2	12/2012	Shelton, IV et al.
8,140,417 B2	3/2012	Shibata	8,322,589 B2	12/2012	Boudreaux
8,141,762 B2	3/2012	Bedi et al.	8,322,590 B2	12/2012	Patel et al.
8,141,763 B2	3/2012	Milliman	8,328,061 B2	12/2012	Kasvikis
8,146,790 B2	4/2012	Milliman	8,328,062 B2	12/2012	Viola
8,152,041 B2	4/2012	Kostrzewski	8,328,063 B2	12/2012	Milliman et al.
8,152,756 B2	4/2012	Webster et al.	8,328,064 B2	12/2012	Racenet et al.
8,157,145 B2	4/2012	Shelton, IV et al.	8,333,313 B2	12/2012	Boudreaux et al.
8,157,148 B2	4/2012	Scirica	8,333,764 B2	12/2012	Francischelli et al.
8,157,151 B2	4/2012	Ingmanson et al.	8,336,753 B2	12/2012	Olson et al.
8,157,152 B2	4/2012	Holsten et al.	8,336,754 B2	12/2012	Cappola et al.
8,157,153 B2	4/2012	Shelton, IV et al.	8,342,378 B2	1/2013	Marczyk et al.
8,161,977 B2	4/2012	Shelton, IV et al.	8,342,379 B2	1/2013	Whitman et al.
8,162,197 B2	4/2012	Mastri et al.	8,348,123 B2	1/2013	Scirica et al.
8,167,185 B2	5/2012	Shelton, IV et al.	8,348,126 B2	1/2013	Olson et al.
8,172,120 B2	5/2012	Boyden et al.	8,348,127 B2	1/2013	Marczyk
8,172,122 B2	5/2012	Kasvikis et al.	8,348,129 B2	1/2013	Bedi et al.
8,172,124 B2	5/2012	Shelton, IV et al.	8,348,130 B2	1/2013	Shah et al.
8,177,797 B2	5/2012	Shimoji et al.	8,348,131 B2	1/2013	Omaits et al.
8,181,840 B2	5/2012	Milliman	8,353,437 B2	1/2013	Boudreaux
8,186,555 B2	5/2012	Shelton, IV et al.	8,353,438 B2	1/2013	Baxter, III et al.
8,186,560 B2	5/2012	Hess et al.	8,353,439 B2	1/2013	Baxter, III et al.
8,191,752 B2	6/2012	Scirica	8,356,740 B1	1/2013	Knodel
8,196,795 B2	6/2012	Moore et al.	8,360,296 B2	1/2013	Zingman
8,196,796 B2	6/2012	Shelton, IV et al.	8,360,297 B2	1/2013	Shelton, IV et al.
8,201,720 B2	6/2012	Hessler	8,360,298 B2	1/2013	Farascioni et al.
8,201,721 B2	6/2012	Zemlok et al.	8,360,299 B2	1/2013	Zemlok et al.
8,205,779 B2	6/2012	Ma et al.	8,365,973 B1	2/2013	White et al.
8,205,780 B2	6/2012	Sorrentino et al.	8,365,975 B1	2/2013	Manoux et al.
8,205,781 B2	6/2012	Baxter, III et al.	8,365,976 B2	2/2013	Hess et al.
8,210,411 B2	7/2012	Yates et al.	8,371,491 B2	2/2013	Huitema et al.
8,210,414 B2	7/2012	Bettuchi et al.	8,371,492 B2	2/2013	Aranyi et al.
8,210,415 B2	7/2012	Ward	8,371,493 B2	2/2013	Aranyi et al.
8,210,416 B2	7/2012	Milliman et al.	8,377,029 B2	2/2013	Nagao et al.
8,214,019 B2	7/2012	Govari et al.	8,393,513 B2	3/2013	Jankowski
8,215,531 B2	7/2012	Shelton, IV et al.	8,393,514 B2	3/2013	Shelton, IV et al.
8,215,533 B2	7/2012	Viola et al.	8,397,971 B2	3/2013	Yates et al.
8,220,688 B2	7/2012	Laurent et al.	8,398,633 B2	3/2013	Mueller
8,220,690 B2	7/2012	Hess et al.	8,403,198 B2	3/2013	Sorrentino et al.
8,231,040 B2	7/2012	Zemlok et al.	8,403,945 B2	3/2013	Whitfield et al.
8,231,042 B2	7/2012	Hessler et al.	8,408,439 B2	4/2013	Huang et al.
8,231,043 B2	7/2012	Tarinelli et al.	8,408,442 B2	4/2013	Racenet et al.
8,236,010 B2	8/2012	Ortiz et al.	8,413,870 B2	4/2013	Pastorelli et al.
8,241,322 B2	8/2012	Whitman et al.	8,413,871 B2	4/2013	Racenet et al.
8,245,898 B2	8/2012	Smith et al.	8,413,872 B2	4/2013	Patel
8,245,899 B2	8/2012	Swensgard et al.	8,414,577 B2	4/2013	Boudreaux et al.
8,245,900 B2	8/2012	Scirica	8,418,909 B2	4/2013	Kostrzewski
8,245,901 B2	8/2012	Stopek	8,424,737 B2	4/2013	Scirica
8,246,637 B2	8/2012	Viola et al.	8,424,739 B2	4/2013	Racenet et al.
			8,424,740 B2	4/2013	Shelton, IV et al.
			8,424,741 B2	4/2013	McGuckin, Jr. et al.
			8,430,292 B2	4/2013	Patel et al.
			8,439,246 B1	5/2013	Knodel



(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,444,036 B2	5/2013	Shelton, IV	8,632,563 B2	1/2014	Nagase et al.
8,453,904 B2	6/2013	Eskaros et al.	8,636,187 B2	1/2014	Hueil et al.
8,453,906 B2	6/2013	Huang et al.	8,636,191 B2	1/2014	Meagher
8,453,907 B2	6/2013	Laurent et al.	8,636,736 B2	1/2014	Yates et al.
8,453,908 B2	6/2013	Bedi et al.	8,652,120 B2	2/2014	Giordano et al.
8,453,912 B2	6/2013	Mastri et al.	8,657,174 B2	2/2014	Yates et al.
8,453,914 B2	6/2013	Laurent et al.	8,657,176 B2	2/2014	Shelton, IV et al.
8,454,628 B2	6/2013	Smith et al.	8,657,177 B2	2/2014	Scirica et al.
8,459,520 B2	6/2013	Giordano et al.	8,657,178 B2	2/2014	Hueil et al.
8,459,525 B2	6/2013	Yates et al.	8,657,821 B2	2/2014	Palermo
8,464,922 B2	6/2013	Marczyk	8,662,370 B2	3/2014	Takei
8,464,923 B2	6/2013	Shelton, IV	8,668,129 B2	3/2014	Olson
8,464,924 B2	6/2013	Gresham et al.	8,668,130 B2	3/2014	Hess et al.
8,464,925 B2	6/2013	Hull et al.	8,672,206 B2	3/2014	Aranyi et al.
8,469,973 B2	6/2013	Meade et al.	8,672,207 B2	3/2014	Shelton, IV et al.
8,470,355 B2	6/2013	Skalla et al.	8,672,208 B2	3/2014	Hess et al.
8,474,677 B2	7/2013	Woodard, Jr. et al.	8,672,951 B2	3/2014	Smith et al.
8,475,454 B1	7/2013	Alshemari	8,678,263 B2	3/2014	Viola
8,479,969 B2	7/2013	Shelton, IV	8,684,250 B2	4/2014	Bettuchi et al.
8,480,703 B2	7/2013	Nicholas et al.	8,684,253 B2	4/2014	Giordano et al.
8,485,412 B2	7/2013	Shelton, IV et al.	8,695,866 B2	4/2014	Leimbach et al.
8,485,413 B2	7/2013	Scheib et al.	8,701,958 B2	4/2014	Shelton, IV et al.
8,490,853 B2	7/2013	Criscuolo et al.	8,701,959 B2	4/2014	Shah
8,496,156 B2	7/2013	Sniffin et al.	8,708,210 B2	4/2014	Zemlok et al.
8,499,992 B2	8/2013	Whitman et al.	8,708,211 B2	4/2014	Zemlok et al.
8,499,993 B2	8/2013	Shelton, IV et al.	8,708,213 B2	4/2014	Shelton, IV et al.
8,506,555 B2	8/2013	Ruiz Morales	8,720,766 B2	5/2014	Hess et al.
8,512,359 B2	8/2013	Whitman et al.	8,721,630 B2	5/2014	Ortiz et al.
8,517,239 B2	8/2013	Scheib et al.	8,727,197 B2	5/2014	Hess et al.
8,517,241 B2	8/2013	Nicholas et al.	8,727,199 B2	5/2014	Wenchell
8,517,243 B2	8/2013	Giordano et al.	8,733,612 B2	5/2014	Ma
8,517,244 B2	8/2013	Shelton, IV et al.	8,733,613 B2	5/2014	Huitema et al.
8,523,043 B2	9/2013	Ullrich et al.	8,733,614 B2	5/2014	Ross et al.
8,529,600 B2	9/2013	Woodard, Jr. et al.	8,734,478 B2	5/2014	Widenhouse et al.
8,529,819 B2	9/2013	Ostapoff et al.	8,740,034 B2	6/2014	Morgan et al.
8,534,528 B2	9/2013	Shelton, IV	8,740,037 B2	6/2014	Shelton, IV et al.
8,540,128 B2	9/2013	Shelton, IV et al.	8,740,038 B2	6/2014	Shelton, IV et al.
8,540,129 B2	9/2013	Baxter, III et al.	8,746,529 B2	6/2014	Shelton, IV et al.
8,540,130 B2	9/2013	Moore et al.	8,746,530 B2	6/2014	Giordano et al.
8,540,131 B2	9/2013	Swayze	8,746,535 B2	6/2014	Shelton, IV et al.
8,540,133 B2	9/2013	Bedi et al.	8,747,238 B2	6/2014	Shelton, IV et al.
8,550,984 B2	10/2013	Takemoto	8,752,699 B2	6/2014	Morgan et al.
8,556,151 B2	10/2013	Viola	8,752,747 B2	6/2014	Shelton, IV et al.
8,561,870 B2	10/2013	Baxter, III et al.	8,752,749 B2	6/2014	Moore et al.
8,561,873 B2	10/2013	Ingmanson et al.	8,757,465 B2	6/2014	Woodard, Jr. et al.
8,567,656 B2	10/2013	Shelton, IV et al.	8,758,391 B2	6/2014	Swayze et al.
8,568,425 B2	10/2013	Ross et al.	8,763,875 B2	7/2014	Morgan et al.
8,573,459 B2	11/2013	Smith et al.	8,763,877 B2	7/2014	Schall et al.
8,573,461 B2	11/2013	Shelton, IV et al.	8,763,879 B2	7/2014	Shelton, IV et al.
8,573,465 B2	11/2013	Shelton, IV	8,770,458 B2	7/2014	Scirica
8,579,176 B2	11/2013	Smith et al.	8,770,459 B2	7/2014	Racenet et al.
8,579,178 B2	11/2013	Holsten et al.	8,770,460 B2	7/2014	Belzer
8,579,937 B2	11/2013	Gresham	8,777,004 B2	7/2014	Shelton, IV et al.
8,584,919 B2	11/2013	Hueil et al.	8,783,541 B2	7/2014	Shelton, IV et al.
8,590,760 B2	11/2013	Cummins et al.	8,783,542 B2	7/2014	Riestenberg et al.
8,590,762 B2	11/2013	Hess et al.	8,783,543 B2	7/2014	Shelton, IV et al.
8,590,764 B2	11/2013	Hartwick et al.	8,789,737 B2	7/2014	Hodgkinson et al.
8,596,513 B2	12/2013	Olson et al.	8,789,739 B2	7/2014	Swensgard
8,602,287 B2	12/2013	Yates et al.	8,789,740 B2	7/2014	Baxter, III et al.
8,602,288 B2	12/2013	Shelton, IV et al.	8,789,741 B2	7/2014	Baxter, III et al.
8,608,043 B2	12/2013	Scirica	8,794,496 B2	8/2014	Scirica
8,608,044 B2	12/2013	Hueil et al.	8,794,497 B2	8/2014	Zingman
8,608,045 B2	12/2013	Smith et al.	8,795,308 B2	8/2014	Valin
8,608,046 B2	12/2013	Laurent et al.	8,800,837 B2	8/2014	Zemlok
8,613,383 B2	12/2013	Beckman et al.	8,800,838 B2	8/2014	Shelton, IV
8,616,431 B2	12/2013	Timm et al.	8,800,840 B2	8/2014	Jankowski
8,622,274 B2	1/2014	Yates et al.	8,800,841 B2	8/2014	Ellerhorst et al.
8,622,275 B2	1/2014	Baxter, III et al.	8,800,841 B2	8/2014	Shelton, IV et al.
8,627,993 B2	1/2014	Smith et al.	8,801,734 B2	8/2014	Shelton, IV et al.
8,627,995 B2	1/2014	Smith et al.	8,801,735 B2	8/2014	Shelton, IV et al.
8,631,987 B2	1/2014	Shelton, IV et al.	8,801,752 B2	8/2014	Fortier et al.
8,631,993 B2	1/2014	Kostrzewski	8,806,973 B2	8/2014	Ross et al.
8,632,462 B2	1/2014	Yoo et al.	8,807,414 B2	8/2014	Ross et al.
8,632,525 B2	1/2014	Kerr et al.	8,808,311 B2	8/2014	Heinrich et al.
8,632,535 B2	1/2014	Shelton, IV et al.	8,808,325 B2	8/2014	Hess et al.
			8,814,024 B2	8/2014	Woodard, Jr. et al.
			8,814,025 B2	8/2014	Miller et al.
			8,820,603 B2	9/2014	Shelton, IV et al.
			8,820,605 B2	9/2014	Shelton, IV
			8,820,606 B2	9/2014	Hodgkinson

(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,827,133 B2	9/2014	Shelton, IV et al.	9,055,944 B2	6/2015	Hodgkinson et al.
8,827,134 B2	9/2014	Viola et al.	9,060,770 B2	6/2015	Shelton, IV et al.
8,827,903 B2	9/2014	Shelton, IV et al.	9,060,894 B2	6/2015	Wubbeling
8,833,632 B2	9/2014	Swensgard	9,072,515 B2	7/2015	Hall et al.
8,840,003 B2	9/2014	Morgan et al.	9,072,535 B2	7/2015	Shelton, IV et al.
8,840,603 B2	9/2014	Shelton, IV et al.	9,072,536 B2	7/2015	Shelton, IV et al.
8,844,789 B2	9/2014	Shelton, IV et al.	9,078,653 B2	7/2015	Leimbach et al.
8,851,354 B2	10/2014	Swensgard et al.	9,084,601 B2	7/2015	Moore et al.
8,857,693 B2	10/2014	Schuckmann et al.	9,084,602 B2	7/2015	Gleiman
8,857,694 B2	10/2014	Shelton, IV et al.	9,089,326 B2	7/2015	Krumanaker et al.
8,858,538 B2	10/2014	Belson et al.	9,089,330 B2	7/2015	Widenhouse et al.
8,858,571 B2	10/2014	Shelton, IV et al.	9,089,352 B2	7/2015	Jeong
8,858,590 B2	10/2014	Shelton, IV et al.	9,095,339 B2	8/2015	Moore et al.
8,864,007 B2	10/2014	Widenhouse et al.	9,095,362 B2	8/2015	Dachs, II et al.
8,864,009 B2	10/2014	Shelton, IV et al.	9,101,358 B2	8/2015	Kerr et al.
8,870,050 B2	10/2014	Hodgkinson	9,101,385 B2	8/2015	Shelton, IV et al.
8,875,971 B2	11/2014	Hall et al.	9,107,663 B2	8/2015	Swensgard
8,875,972 B2	11/2014	Weisenburgh, II et al.	9,113,862 B2	8/2015	Morgan et al.
8,876,857 B2	11/2014	Burbank	9,113,864 B2	8/2015	Morgan et al.
8,893,946 B2	11/2014	Boudreaux et al.	9,113,865 B2	8/2015	Shelton, IV et al.
8,893,949 B2	11/2014	Shelton, IV et al.	9,113,874 B2	8/2015	Shelton, IV et al.
8,894,647 B2	11/2014	Beardsley et al.	9,113,880 B2	8/2015	Zemlok et al.
8,899,463 B2	12/2014	Schall et al.	9,113,883 B2	8/2015	Aronhalt et al.
8,899,464 B2	12/2014	Hueil et al.	9,113,884 B2	8/2015	Shelton, IV et al.
8,899,465 B2	12/2014	Shelton, IV et al.	9,119,957 B2	9/2015	Gantz et al.
8,899,466 B2	12/2014	Baxter, III et al.	9,125,654 B2	9/2015	Aronhalt et al.
8,905,977 B2	12/2014	Shelton et al.	9,125,662 B2	9/2015	Shelton, IV
8,911,471 B2	12/2014	Spivey et al.	9,131,940 B2	9/2015	Huitema et al.
8,920,433 B2	12/2014	Barrier et al.	9,138,225 B2	9/2015	Huang et al.
8,920,435 B2	12/2014	Smith et al.	9,149,274 B2	10/2015	Spivey et al.
8,920,443 B2	12/2014	Hiles et al.	9,168,038 B2	10/2015	Shelton, IV et al.
8,925,782 B2	1/2015	Shelton, IV	9,179,911 B2	11/2015	Morgan et al.
8,925,783 B2	1/2015	Zemlok et al.	9,179,912 B2	11/2015	Yates et al.
8,925,788 B2	1/2015	Hess et al.	9,186,143 B2	11/2015	Timm et al.
8,926,598 B2	1/2015	Mollere et al.	9,192,380 B2	11/2015	(Tarinelli) Racenet et al.
8,931,682 B2	1/2015	Timm et al.	9,192,384 B2	11/2015	Bettuchi
8,939,343 B2	1/2015	Milliman et al.	9,198,661 B2	12/2015	Swensgard
8,939,344 B2	1/2015	Olson et al.	9,198,662 B2	12/2015	Barton et al.
8,945,163 B2	2/2015	Voegele et al.	9,204,877 B2	12/2015	Whitman et al.
8,956,390 B2	2/2015	Shah et al.	9,204,878 B2	12/2015	Hall et al.
8,960,520 B2	2/2015	McCuen	9,204,879 B2	12/2015	Shelton, IV
8,960,521 B2	2/2015	Kostrzewski	9,204,880 B2	12/2015	Baxter, III et al.
8,967,443 B2	3/2015	McCuen	9,211,120 B2	12/2015	Scheib et al.
8,967,446 B2	3/2015	Beardsley et al.	9,211,121 B2	12/2015	Hall et al.
8,967,448 B2	3/2015	Carter et al.	9,211,122 B2	12/2015	Hagerty et al.
8,973,803 B2	3/2015	Hall et al.	9,216,019 B2	12/2015	Schmid et al.
8,973,804 B2	3/2015	Hess et al.	9,220,500 B2	12/2015	Swayze et al.
8,974,440 B2	3/2015	Farritor et al.	9,220,501 B2	12/2015	Baxter, III et al.
8,978,954 B2	3/2015	Shelton, IV et al.	9,220,502 B2	12/2015	Zemlok et al.
8,978,955 B2	3/2015	Aronhalt et al.	9,220,559 B2	12/2015	Worrell et al.
8,978,956 B2	3/2015	Schall et al.	9,226,751 B2	1/2016	Shelton, IV et al.
8,985,428 B2	3/2015	Natarajan et al.	9,232,941 B2	1/2016	Mandakolathur Vasudevan et al.
8,991,676 B2	3/2015	Hess et al.	9,232,945 B2	1/2016	Zingman
8,991,677 B2	3/2015	Moore et al.	9,237,891 B2	1/2016	Shelton, IV
8,992,422 B2	3/2015	Spivey et al.	9,241,714 B2	1/2016	Timm et al.
8,998,058 B2	4/2015	Moore et al.	9,271,799 B2	3/2016	Shelton, IV et al.
8,998,059 B2	4/2015	Smith et al.	9,272,406 B2	3/2016	Aronhalt et al.
9,005,230 B2	4/2015	Yates et al.	9,277,919 B2	3/2016	Timmer et al.
9,005,238 B2	4/2015	DeSantis et al.	9,282,962 B2	3/2016	Schmid et al.
9,010,608 B2	4/2015	Casasanta, Jr. et al.	9,282,966 B2	3/2016	Shelton, IV et al.
9,016,541 B2	4/2015	Viola et al.	9,282,974 B2	3/2016	Shelton, IV
9,016,542 B2	4/2015	Shelton, IV et al.	9,283,054 B2	3/2016	Morgan et al.
9,028,494 B2	5/2015	Shelton, IV et al.	9,289,206 B2	3/2016	Hess et al.
9,028,495 B2	5/2015	Mueller et al.	9,289,210 B2	3/2016	Baxter, III et al.
9,028,519 B2	5/2015	Yates et al.	9,289,212 B2	3/2016	Shelton, IV et al.
9,033,203 B2	5/2015	Woodard, Jr. et al.	9,289,225 B2	3/2016	Shelton, IV et al.
9,033,204 B2	5/2015	Shelton, IV et al.	9,289,256 B2	3/2016	Shelton, IV et al.
9,038,881 B1	5/2015	Schaller et al.	9,295,464 B2	3/2016	Shelton, IV et al.
9,044,227 B2	6/2015	Shelton, IV et al.	9,295,466 B2	3/2016	Hodgkinson et al.
9,044,228 B2	6/2015	Woodard, Jr. et al.	9,295,784 B2	3/2016	Eggert et al.
9,044,229 B2	6/2015	Scheib et al.	9,301,752 B2	4/2016	Mandakolathur Vasudevan et al.
9,044,230 B2	6/2015	Morgan et al.	9,301,753 B2	4/2016	Aldridge et al.
9,050,083 B2	6/2015	Yates et al.	9,301,755 B2	4/2016	Shelton, IV et al.
9,050,084 B2	6/2015	Schmid et al.	9,301,759 B2	4/2016	Spivey et al.
9,055,941 B2	6/2015	Schmid et al.	9,307,965 B2	4/2016	Ming et al.
			9,307,986 B2	4/2016	Hall et al.
			9,307,987 B2	4/2016	Swensgard et al.
			9,307,988 B2	4/2016	Shelton, IV
			9,307,989 B2	4/2016	Shelton, IV et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

9,307,994 B2	4/2016	Gresham et al.	9,585,662 B2	3/2017	Shelton, IV et al.
9,314,246 B2	4/2016	Shelton, IV et al.	9,592,050 B2	3/2017	Schmid et al.
9,314,247 B2	4/2016	Shelton, IV et al.	9,592,052 B2	3/2017	Shelton, IV
9,320,518 B2	4/2016	Henderson et al.	9,592,053 B2	3/2017	Shelton, IV et al.
9,320,520 B2	4/2016	Shelton, IV et al.	9,592,054 B2	3/2017	Schmid et al.
9,320,521 B2	4/2016	Shelton, IV et al.	9,597,075 B2	3/2017	Shelton, IV et al.
9,320,523 B2	4/2016	Shelton, IV et al.	9,597,080 B2	3/2017	Milliman et al.
9,326,767 B2	5/2016	Koch et al.	9,603,595 B2	3/2017	Shelton, IV et al.
9,326,768 B2	5/2016	Shelton, IV	9,603,598 B2	3/2017	Shelton, IV et al.
9,326,769 B2	5/2016	Shelton, IV et al.	9,603,991 B2	3/2017	Shelton, IV et al.
9,326,770 B2	5/2016	Shelton, IV et al.	9,615,826 B2	4/2017	Shelton, IV et al.
9,326,771 B2	5/2016	Baxter, III et al.	9,629,623 B2	4/2017	Lytle, IV et al.
9,332,974 B2	5/2016	Henderson et al.	9,629,626 B2	4/2017	Soltz et al.
9,332,984 B2	5/2016	Weaner et al.	9,629,629 B2	4/2017	Leimbach et al.
9,332,987 B2	5/2016	Leimbach et al.	9,629,814 B2	4/2017	Widenhouse et al.
9,345,477 B2	5/2016	Anim et al.	9,642,620 B2	5/2017	Baxter, III et al.
9,345,481 B2	5/2016	Hall et al.	9,649,096 B2	5/2017	Sholev
9,351,726 B2	5/2016	Leimbach et al.	9,649,110 B2	5/2017	Parihar et al.
9,351,727 B2	5/2016	Leimbach et al.	9,649,111 B2	5/2017	Shelton, IV et al.
9,351,730 B2	5/2016	Schmid et al.	9,655,614 B2	5/2017	Swensgard et al.
9,351,731 B2	5/2016	Carter et al.	9,655,615 B2	5/2017	Knodel et al.
9,358,003 B2	6/2016	Hall et al.	9,655,624 B2	5/2017	Shelton, IV et al.
9,358,005 B2	6/2016	Shelton, IV et al.	9,662,110 B2	5/2017	Huang et al.
9,364,219 B2	6/2016	Olson et al.	9,668,732 B2	6/2017	Patel et al.
9,364,229 B2	6/2016	D'Agostino et al.	9,675,351 B2	6/2017	Hodgkinson et al.
9,364,230 B2	6/2016	Shelton, IV et al.	9,675,355 B2	6/2017	Shelton, IV et al.
9,364,233 B2	6/2016	Alexander, III et al.	9,675,372 B2	6/2017	Laurent et al.
9,370,358 B2	6/2016	Shelton, IV et al.	9,675,375 B2	6/2017	Houser et al.
9,370,364 B2	6/2016	Smith et al.	9,681,870 B2	6/2017	Baxter, III et al.
9,386,983 B2	7/2016	Swensgard et al.	9,681,873 B2	6/2017	Smith et al.
9,386,984 B2	7/2016	Aronhalt et al.	9,687,230 B2	6/2017	Leimbach et al.
9,386,985 B2	7/2016	Koch, Jr. et al.	9,687,231 B2	6/2017	Baxter, III et al.
9,386,988 B2	7/2016	Baxter, III et al.	9,687,232 B2	6/2017	Shelton, IV et al.
9,393,015 B2	7/2016	Laurent et al.	9,687,236 B2	6/2017	Leimbach et al.
9,393,018 B2	7/2016	Wang et al.	9,687,237 B2	6/2017	Schmid et al.
9,398,911 B2	7/2016	Auld	9,690,362 B2	6/2017	Leimbach et al.
9,402,626 B2	8/2016	Ortiz et al.	9,693,772 B2	7/2017	Ingmanson et al.
9,408,604 B2	8/2016	Shelton, IV et al.	9,693,777 B2	7/2017	Schellin et al.
9,408,606 B2	8/2016	Shelton, IV	9,693,819 B2	7/2017	Francischelli et al.
9,414,838 B2	8/2016	Shelton, IV et al.	9,700,309 B2	7/2017	Jaworek et al.
9,421,014 B2	8/2016	Ingmanson et al.	9,700,310 B2	7/2017	Morgan et al.
9,421,060 B2	8/2016	Monson et al.	9,700,317 B2	7/2017	Aronhalt et al.
9,427,223 B2	8/2016	Park et al.	9,700,319 B2	7/2017	Motooka et al.
9,433,411 B2	9/2016	Racenet et al.	9,700,321 B2	7/2017	Shelton, IV et al.
9,433,419 B2	9/2016	Gonzalez et al.	9,706,991 B2	7/2017	Hess et al.
9,433,420 B2	9/2016	Hodgkinson	9,724,091 B2	8/2017	Shelton, IV et al.
9,439,649 B2	9/2016	Shelton, IV et al.	9,724,092 B2	8/2017	Baxter, III et al.
9,439,651 B2	9/2016	Smith et al.	9,724,094 B2	8/2017	Baber et al.
9,445,813 B2	9/2016	Shelton, IV et al.	9,724,098 B2	8/2017	Baxter, III et al.
9,451,958 B2	9/2016	Shelton, IV et al.	9,730,692 B2	8/2017	Shelton, IV et al.
9,468,438 B2	10/2016	Baber et al.	9,730,695 B2	8/2017	Leimbach et al.
9,480,476 B2	11/2016	Aldridge et al.	9,730,697 B2	8/2017	Morgan et al.
9,486,213 B2	11/2016	Altman et al.	9,733,663 B2	8/2017	Leimbach et al.
9,486,214 B2	11/2016	Shelton, IV	9,737,301 B2	8/2017	Baber et al.
9,486,302 B2	11/2016	Boey et al.	9,737,303 B2	8/2017	Shelton, IV et al.
9,492,167 B2	11/2016	Shelton, IV et al.	9,743,928 B2	8/2017	Shelton, IV et al.
9,492,170 B2	11/2016	Bear et al.	9,743,929 B2	8/2017	Leimbach et al.
9,498,219 B2	11/2016	Moore et al.	9,750,498 B2	9/2017	Timm et al.
9,510,828 B2	12/2016	Yates et al.	9,750,499 B2	9/2017	Leimbach et al.
9,510,830 B2	12/2016	Shelton, IV et al.	9,757,123 B2	9/2017	Giordano et al.
9,510,925 B2	12/2016	Hotter et al.	9,757,124 B2	9/2017	Schellin et al.
9,517,063 B2	12/2016	Swayze et al.	9,757,128 B2	9/2017	Baber et al.
9,517,068 B2	12/2016	Shelton, IV et al.	9,757,130 B2	9/2017	Shelton, IV
9,522,029 B2	12/2016	Yates et al.	9,763,662 B2	9/2017	Shelton, IV et al.
9,549,732 B2	1/2017	Yates et al.	9,770,245 B2	9/2017	Swayze et al.
9,549,735 B2	1/2017	Shelton, IV et al.	9,775,608 B2	10/2017	Aronhalt et al.
9,554,794 B2	1/2017	Baber et al.	9,775,609 B2	10/2017	Shelton, IV et al.
9,561,032 B2	2/2017	Shelton, IV et al.	9,775,613 B2	10/2017	Shelton, IV et al.
9,561,038 B2	2/2017	Shelton, IV et al.	9,775,614 B2	10/2017	Shelton, IV et al.
9,566,061 B2	2/2017	Aronhalt et al.	9,782,169 B2	10/2017	Kimsey et al.
9,572,574 B2	2/2017	Shelton, IV et al.	9,788,834 B2	10/2017	Schmid et al.
9,572,577 B2	2/2017	Lloyd et al.	9,788,836 B2	10/2017	Overmyer et al.
9,574,644 B2	2/2017	Parihar	9,795,382 B2	10/2017	Shelton, IV
9,585,657 B2	3/2017	Shelton, IV et al.	9,795,384 B2	10/2017	Weaner et al.
9,585,660 B2	3/2017	Laurent et al.	9,801,626 B2	10/2017	Parihar et al.
			9,801,627 B2	10/2017	Harris et al.
			9,801,628 B2	10/2017	Harris et al.
			9,801,634 B2	10/2017	Shelton, IV et al.
			9,804,618 B2	10/2017	Leimbach et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,808,244 B2	11/2017	Leimbach et al.	10,070,863 B2	9/2018	Swayze et al.
9,808,247 B2	11/2017	Shelton, IV et al.	10,071,452 B2	9/2018	Shelton, IV et al.
9,808,249 B2	11/2017	Shelton, IV	10,076,325 B2	9/2018	Huang et al.
9,814,460 B2	11/2017	Kimsey et al.	10,085,806 B2	10/2018	Hagn et al.
9,814,462 B2	11/2017	Woodard, Jr. et al.	10,111,679 B2	10/2018	Baber et al.
9,820,738 B2	11/2017	Lytle, IV et al.	10,123,798 B2	11/2018	Baxter, III et al.
9,820,741 B2	11/2017	Kostrzewski	10,130,352 B2	11/2018	Widenhouse et al.
9,826,976 B2	11/2017	Parihar et al.	10,130,359 B2	11/2018	Hess et al.
9,826,977 B2	11/2017	Leimbach et al.	10,130,363 B2	11/2018	Huitema et al.
9,826,978 B2	11/2017	Shelton, IV et al.	10,130,366 B2	11/2018	Shelton, IV et al.
9,833,236 B2	12/2017	Shelton, IV et al.	10,135,242 B2	11/2018	Baber et al.
9,833,241 B2	12/2017	Huitema et al.	10,136,887 B2	11/2018	Shelton, IV et al.
9,839,420 B2	12/2017	Shelton, IV et al.	10,136,890 B2	11/2018	Shelton, IV et al.
9,839,421 B2	12/2017	Zerkle et al.	10,149,679 B2	12/2018	Shelton, IV et al.
9,839,422 B2	12/2017	Schellin et al.	10,149,680 B2	12/2018	Parihar et al.
9,839,423 B2	12/2017	Vendely et al.	10,149,682 B2	12/2018	Shelton, IV et al.
9,839,427 B2	12/2017	Swayze et al.	10,159,482 B2	12/2018	Swayze et al.
9,839,428 B2	12/2017	Baxter, III et al.	10,166,025 B2	1/2019	Leimbach et al.
9,839,429 B2	12/2017	Weisenburgh, II et al.	10,172,616 B2	1/2019	Murray et al.
9,844,368 B2	12/2017	Boudreaux et al.	10,182,819 B2	1/2019	Shelton, IV
9,844,369 B2	12/2017	Huitema et al.	10,188,393 B2	1/2019	Smith et al.
9,844,372 B2	12/2017	Shelton, IV et al.	10,194,910 B2	2/2019	Shelton, IV et al.
9,844,373 B2	12/2017	Swayze et al.	10,201,364 B2	2/2019	Leimbach et al.
9,844,376 B2	12/2017	Baxter, III et al.	10,206,677 B2	2/2019	Harris et al.
9,848,873 B2	12/2017	Shelton, IV	10,206,678 B2	2/2019	Shelton, IV et al.
9,848,875 B2	12/2017	Aronhalt et al.	10,213,198 B2	2/2019	Aronhalt et al.
9,861,359 B2	1/2018	Shelton, IV et al.	10,238,385 B2	3/2019	Yates et al.
9,861,361 B2	1/2018	Aronhalt et al.	10,238,387 B2	3/2019	Yates et al.
9,867,612 B2	1/2018	Parihar et al.	10,245,035 B2	4/2019	Swayze et al.
9,867,618 B2	1/2018	Hall et al.	10,258,330 B2	4/2019	Shelton, IV et al.
9,872,684 B2	1/2018	Hall et al.	10,258,333 B2	4/2019	Shelton, IV et al.
9,877,721 B2	1/2018	Schellin et al.	10,265,065 B2	4/2019	Shelton, IV et al.
9,883,860 B2	2/2018	Leimbach	10,265,067 B2	4/2019	Yates et al.
9,883,861 B2	2/2018	Shelton, IV et al.	10,265,072 B2	4/2019	Shelton, IV et al.
9,884,456 B2	2/2018	Schellin et al.	10,271,845 B2	4/2019	Shelton, IV
9,888,919 B2	2/2018	Leimbach et al.	10,299,792 B2	5/2019	Huitema et al.
9,888,924 B2	2/2018	Ebersole et al.	10,327,764 B2	6/2019	Harris et al.
9,895,147 B2	2/2018	Shelton, IV	10,327,776 B2	6/2019	Harris et al.
9,913,642 B2	3/2018	Leimbach et al.	10,335,144 B2	7/2019	Shelton, IV et al.
9,913,647 B2	3/2018	Weisenburgh, II et al.	10,335,148 B2	7/2019	Shelton, IV et al.
9,918,704 B2	3/2018	Shelton, IV et al.	10,335,150 B2	7/2019	Shelton, IV
9,918,716 B2	3/2018	Baxter, III et al.	10,342,533 B2	7/2019	Shelton, IV et al.
9,924,942 B2	3/2018	Swayze et al.	10,342,541 B2	7/2019	Shelton, IV et al.
9,924,944 B2	3/2018	Shelton, IV et al.	10,383,629 B2	8/2019	Ross et al.
9,924,947 B2	3/2018	Shelton, IV et al.	10,390,823 B2	8/2019	Shelton, IV et al.
9,943,310 B2	4/2018	Harris et al.	10,398,433 B2	9/2019	Boudreaux et al.
9,962,158 B2	5/2018	Hall et al.	10,398,436 B2	9/2019	Shelton, IV et al.
9,962,161 B2	5/2018	Scheib et al.	10,405,854 B2	9/2019	Schmid et al.
9,968,354 B2	5/2018	Shelton, IV et al.	10,405,857 B2	9/2019	Shelton, IV et al.
9,968,356 B2	5/2018	Shelton, IV et al.	10,426,476 B2	10/2019	Harris et al.
9,974,529 B2	5/2018	Shelton, IV et al.	10,426,477 B2	10/2019	Harris et al.
9,974,538 B2	5/2018	Baxter, III et al.	10,426,478 B2	10/2019	Shelton, IV et al.
9,980,713 B2	5/2018	Aronhalt et al.	10,433,918 B2	10/2019	Shelton, IV et al.
9,987,006 B2	6/2018	Morgan et al.	10,441,285 B2	10/2019	Shelton, IV et al.
9,999,408 B2	6/2018	Boudreaux et al.	10,441,369 B2	10/2019	Shelton, IV et al.
10,004,497 B2	6/2018	Overmyer et al.	10,456,133 B2	10/2019	Yates et al.
10,004,498 B2	6/2018	Morgan et al.	10,470,762 B2	11/2019	Leimbach et al.
10,010,322 B2	7/2018	Shelton, IV et al.	10,470,763 B2	11/2019	Yates et al.
10,010,324 B2	7/2018	Huitema et al.	10,470,768 B2	11/2019	Harris et al.
10,013,049 B2	7/2018	Leimbach et al.	10,485,536 B2	11/2019	Ming et al.
10,016,199 B2	7/2018	Baber et al.	10,492,787 B2	12/2019	Smith et al.
10,028,742 B2	7/2018	Shelton, IV et al.	10,517,594 B2	12/2019	Shelton, IV et al.
10,028,743 B2	7/2018	Shelton, IV et al.	10,517,682 B2	12/2019	Giordano et al.
10,028,761 B2	7/2018	Leimbach et al.	2002/0117534 A1	8/2002	Green et al.
10,039,529 B2	8/2018	Kerr et al.	2002/0143346 A1*	10/2002	McGuckin, Jr. ....
10,045,769 B2	8/2018	Aronhalt et al.			A61B 17/07207
10,045,781 B2	8/2018	Cropper et al.			606/139
10,052,099 B2	8/2018	Morgan et al.	2003/0009193 A1	1/2003	Corsaro
10,052,100 B2	8/2018	Morgan et al.	2003/0039689 A1	2/2003	Chen et al.
10,052,104 B2	8/2018	Shelton, IV et al.	2003/0096158 A1	5/2003	Takano et al.
10,058,327 B2	8/2018	Weisenburgh, II et al.	2003/0181900 A1	9/2003	Long
10,058,963 B2	8/2018	Shelton, IV et al.	2003/0236505 A1	12/2003	Bonadio et al.
10,064,621 B2	9/2018	Kerr et al.	2004/0068161 A1	4/2004	Couvillon
10,064,624 B2	9/2018	Shelton, IV et al.	2004/0068224 A1	4/2004	Couvillon et al.
10,070,861 B2	9/2018	Spivey et al.	2004/0102783 A1	5/2004	Sutterlin et al.
			2004/0108357 A1	6/2004	Milliman et al.
			2004/0147909 A1	7/2004	Johnston et al.
			2004/0164123 A1	8/2004	Racenet et al.
			2004/0199181 A1	10/2004	Knodel et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2004/0222268	A1	11/2004	Bilotti et al.	2009/0204108	A1	8/2009	Steffen
2004/0225186	A1	11/2004	Horne et al.	2009/0206125	A1	8/2009	Huitema et al.
2004/0232201	A1	11/2004	Wenchell et al.	2009/0206126	A1	8/2009	Huitema et al.
2005/0054946	A1	3/2005	Krzyzanowski	2009/0206131	A1	8/2009	Weisenburgh, II et al.
2005/0070929	A1	3/2005	Dalessandro et al.	2009/0206133	A1	8/2009	Morgan et al.
2005/0080342	A1	4/2005	Gilreath et al.	2009/0206137	A1	8/2009	Hall et al.
2005/0125897	A1	6/2005	Wyslucha et al.	2009/0206139	A1	8/2009	Hall et al.
2005/0139636	A1	6/2005	Schwemberger et al.	2009/0206141	A1	8/2009	Huitema et al.
2005/0143759	A1	6/2005	Kelly	2009/0206142	A1	8/2009	Huitema et al.
2005/0184121	A1	8/2005	Heinrich	2009/0242610	A1	10/2009	Shelton, IV et al.
2005/0228224	A1	10/2005	Okada et al.	2009/0255974	A1	10/2009	Viola
2005/0263563	A1	12/2005	Racenet et al.	2009/0308907	A1	12/2009	Nalagatla et al.
2006/0049229	A1	3/2006	Milliman et al.	2010/0069942	A1	3/2010	Shelton, IV
2006/0089535	A1	4/2006	Raz et al.	2010/0133317	A1	6/2010	Shelton, IV et al.
2006/0173470	A1	8/2006	Oray et al.	2010/0147921	A1	6/2010	Olson
2006/0180634	A1	8/2006	Shelton et al.	2010/0147922	A1	6/2010	Olson
2006/0201989	A1	9/2006	Ojeda	2010/0193566	A1	8/2010	Scheib et al.
2006/0235368	A1	10/2006	Oz	2010/0222901	A1	9/2010	Swayze et al.
2006/0271102	A1	11/2006	Bosshard et al.	2011/0006101	A1	1/2011	Hall et al.
2006/0287576	A1	12/2006	Tsuji et al.	2011/0011916	A1	1/2011	Levine
2006/0289602	A1	12/2006	Wales et al.	2011/0024477	A1	2/2011	Hall
2006/0291981	A1	12/2006	Viola et al.	2011/0024478	A1	2/2011	Shelton, IV
2007/0027468	A1	2/2007	Wales et al.	2011/0036891	A1	2/2011	Zemlok et al.
2007/0051375	A1	3/2007	Milliman	2011/0060363	A1	3/2011	Hess et al.
2007/0084897	A1	4/2007	Shelton et al.	2011/0087276	A1	4/2011	Bedi et al.
2007/0093869	A1	4/2007	Bloom et al.	2011/0091515	A1	4/2011	Zilberman et al.
2007/0102472	A1	5/2007	Shelton	2011/0114697	A1	5/2011	Baxter, III et al.
2007/0106317	A1	5/2007	Shelton et al.	2011/0125176	A1	5/2011	Yates et al.
2007/0134251	A1	6/2007	Ashkenazi et al.	2011/0147433	A1	6/2011	Shelton, IV et al.
2007/0170225	A1	7/2007	Shelton et al.	2011/0163146	A1	7/2011	Ortiz et al.
2007/0173687	A1	7/2007	Shima et al.	2011/0174861	A1	7/2011	Shelton, IV et al.
2007/0175950	A1	8/2007	Shelton et al.	2011/0192882	A1	8/2011	Hess et al.
2007/0175951	A1	8/2007	Shelton et al.	2011/0275901	A1	11/2011	Shelton, IV
2007/0175955	A1	8/2007	Shelton et al.	2011/0276083	A1	11/2011	Shelton, IV et al.
2007/0194079	A1	8/2007	Hueil et al.	2011/0278343	A1	11/2011	Knodel et al.
2007/0194082	A1	8/2007	Morgan et al.	2011/0290856	A1	12/2011	Shelton, IV et al.
2007/0203510	A1	8/2007	Bettuchi	2011/0293690	A1	12/2011	Griffin et al.
2007/0225562	A1	9/2007	Spivey et al.	2011/0295295	A1	12/2011	Shelton, IV et al.
2007/0233163	A1	10/2007	Bombard et al.	2012/0029272	A1	2/2012	Shelton, IV et al.
2007/0246505	A1	10/2007	Pace-Florida et al.	2012/0074200	A1	3/2012	Schmid et al.
2007/0276409	A1	11/2007	Ortiz et al.	2012/0080336	A1	4/2012	Shelton, IV et al.
2007/0279011	A1	12/2007	Jones et al.	2012/0080344	A1	4/2012	Shelton, IV
2008/0029570	A1	2/2008	Shelton et al.	2012/0080478	A1	4/2012	Morgan et al.
2008/0029573	A1	2/2008	Shelton et al.	2012/0080498	A1	4/2012	Shelton, IV et al.
2008/0029574	A1	2/2008	Shelton et al.	2012/0109186	A1	5/2012	Parrott et al.
2008/0029575	A1	2/2008	Shelton et al.	2012/0125792	A1	5/2012	Cassivi
2008/0078802	A1	4/2008	Hess et al.	2012/0175398	A1	7/2012	Sandborn et al.
2008/0082125	A1	4/2008	Murray et al.	2012/0234895	A1	9/2012	O'Connor et al.
2008/0082126	A1	4/2008	Murray et al.	2012/0234897	A1	9/2012	Shelton, IV et al.
2008/0086078	A1	4/2008	Powell et al.	2012/0248169	A1	10/2012	Widenhouse et al.
2008/0091072	A1	4/2008	Omori et al.	2012/0283707	A1	11/2012	Giordano et al.
2008/0108443	A1	5/2008	Jinno et al.	2012/0292367	A1	11/2012	Morgan et al.
2008/0135600	A1	6/2008	Hiranuma et al.	2012/0298722	A1	11/2012	Hess et al.
2008/0140115	A1	6/2008	Stopek	2012/0303002	A1	11/2012	Chowaniec et al.
2008/0169328	A1	7/2008	Shelton	2013/0006227	A1	1/2013	Takashino
2008/0169332	A1	7/2008	Shelton et al.	2013/0020375	A1	1/2013	Shelton, IV et al.
2008/0169333	A1	7/2008	Shelton et al.	2013/0020376	A1	1/2013	Shelton, IV et al.
2008/0172087	A1	7/2008	Fuchs et al.	2013/0023861	A1	1/2013	Shelton, IV et al.
2008/0190989	A1	8/2008	Crews et al.	2013/0026208	A1	1/2013	Shelton, IV et al.
2008/0197167	A1	8/2008	Viola et al.	2013/0026210	A1	1/2013	Shelton, IV et al.
2008/0200762	A1	8/2008	Stokes et al.	2013/0087597	A1	4/2013	Shelton, IV et al.
2008/0249536	A1	10/2008	Stahler et al.	2013/0098970	A1	4/2013	Racenet et al.
2008/0296346	A1	12/2008	Shelton, IV et al.	2013/0116669	A1	5/2013	Shelton, IV et al.
2008/0308602	A1	12/2008	Timm et al.	2013/0153641	A1	6/2013	Shelton, IV et al.
2008/0308603	A1	12/2008	Shelton et al.	2013/0175317	A1	7/2013	Yates et al.
2008/0315829	A1	12/2008	Jones et al.	2013/0214025	A1	8/2013	Zemlok et al.
2009/0001121	A1	1/2009	Hess et al.	2013/0233906	A1	9/2013	Hess et al.
2009/0001130	A1	1/2009	Hess et al.	2013/0256373	A1	10/2013	Schmid et al.
2009/0005809	A1	1/2009	Hess et al.	2013/0256380	A1	10/2013	Schmid et al.
2009/0048589	A1	2/2009	Takashino et al.	2013/0270322	A1	10/2013	Scheib et al.
2009/0078736	A1	3/2009	Van Lue	2013/0334283	A1	12/2013	Swayze et al.
2009/0090763	A1	4/2009	Zemlok et al.	2013/0334285	A1	12/2013	Swayze et al.
2009/0099876	A1	4/2009	Whitman	2013/0341374	A1	12/2013	Shelton, IV et al.
2009/0149871	A9	6/2009	Kagan et al.	2014/0001231	A1	1/2014	Shelton, IV et al.
2009/0188964	A1	7/2009	Orlov	2014/0001234	A1	1/2014	Shelton, IV et al.
				2014/0005640	A1	1/2014	Shelton, IV et al.
				2014/0005678	A1	1/2014	Shelton, IV et al.
				2014/0005718	A1	1/2014	Shelton, IV et al.
				2014/0012299	A1	1/2014	Stoddard et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2014/0014705 A1 1/2014 Baxter, III  
 2014/0039549 A1 2/2014 Belsky et al.  
 2014/0048580 A1 2/2014 Merchant et al.  
 2014/0107640 A1 4/2014 Yates et al.  
 2014/0151433 A1 6/2014 Shelton, IV et al.  
 2014/0166724 A1 6/2014 Schellin et al.  
 2014/0166725 A1 6/2014 Schellin et al.  
 2014/0166726 A1 6/2014 Schellin et al.  
 2014/0175152 A1 6/2014 Hess et al.  
 2014/0188159 A1 7/2014 Steege  
 2014/0224857 A1 8/2014 Schmid  
 2014/0243865 A1 8/2014 Swayze et al.  
 2014/0246475 A1 9/2014 Hall et al.  
 2014/0249557 A1 9/2014 Koch et al.  
 2014/0263541 A1 9/2014 Leimbach et al.  
 2014/0263552 A1 9/2014 Hall et al.  
 2014/0263558 A1 9/2014 Hausen et al.  
 2014/0284371 A1 9/2014 Morgan et al.  
 2014/0291379 A1 10/2014 Schellin et al.  
 2014/0291383 A1 10/2014 Spivey et al.  
 2014/0299648 A1 10/2014 Shelton, IV et al.  
 2014/0303645 A1 10/2014 Morgan et al.  
 2014/0330161 A1 11/2014 Swayze et al.  
 2015/0008248 A1 1/2015 Giordano et al.  
 2015/0053737 A1 2/2015 Leimbach et al.  
 2015/0053742 A1 2/2015 Shelton, IV et al.  
 2015/0053743 A1 2/2015 Yates et al.  
 2015/0053746 A1 2/2015 Shelton, IV et al.  
 2015/0053748 A1 2/2015 Yates et al.  
 2015/0060518 A1 3/2015 Shelton, IV et al.  
 2015/0060519 A1 3/2015 Shelton, IV et al.  
 2015/0060520 A1 3/2015 Shelton, IV et al.  
 2015/0060521 A1 3/2015 Weisenburgh, II et al.  
 2015/0076208 A1 3/2015 Shelton, IV  
 2015/0076209 A1 3/2015 Shelton, IV et al.  
 2015/0076210 A1 3/2015 Shelton, IV et al.  
 2015/0076212 A1 3/2015 Shelton, IV  
 2015/0080868 A1 3/2015 Kerr  
 2015/0083781 A1 3/2015 Giordano et al.  
 2015/0083782 A1 3/2015 Scheib et al.  
 2015/0090760 A1 4/2015 Giordano et al.  
 2015/0090762 A1 4/2015 Giordano et al.  
 2015/0173749 A1 6/2015 Shelton, IV et al.  
 2015/0173756 A1 6/2015 Baxter, III et al.  
 2015/0173789 A1 6/2015 Baxter, III et al.  
 2015/0196295 A1 7/2015 Shelton, IV et al.  
 2015/0196296 A1 7/2015 Swayze et al.  
 2015/0196299 A1 7/2015 Swayze et al.  
 2015/0201932 A1 7/2015 Swayze et al.  
 2015/0201936 A1 7/2015 Swayze et al.  
 2015/0201937 A1 7/2015 Swayze et al.  
 2015/0201938 A1 7/2015 Swayze et al.  
 2015/0201939 A1 7/2015 Swayze et al.  
 2015/0201940 A1 7/2015 Swayze et al.  
 2015/0201941 A1 7/2015 Swayze et al.  
 2015/0231409 A1 8/2015 Racenet et al.  
 2015/0272557 A1 10/2015 Overmyer et al.  
 2015/0272571 A1 10/2015 Leimbach et al.  
 2015/0272580 A1 10/2015 Leimbach et al.  
 2015/0272582 A1 10/2015 Leimbach et al.  
 2015/0297222 A1 10/2015 Huitema et al.  
 2015/0297223 A1 10/2015 Huitema et al.  
 2015/0297225 A1 10/2015 Huitema et al.  
 2015/0297228 A1 10/2015 Huitema et al.  
 2015/0297229 A1 10/2015 Schellin et al.  
 2015/0297233 A1 10/2015 Huitema et al.  
 2015/0297234 A1 10/2015 Schellin et al.  
 2015/0313594 A1 11/2015 Shelton, IV et al.  
 2015/0374369 A1 12/2015 Yates et al.  
 2015/0374378 A1 12/2015 Giordano et al.  
 2016/0000431 A1 1/2016 Giordano et al.  
 2016/0000437 A1 1/2016 Giordano et al.  
 2016/0000438 A1 1/2016 Swayze et al.  
 2016/0000442 A1 1/2016 Shelton, IV  
 2016/0000452 A1 1/2016 Yates et al.

2016/0000453 A1 1/2016 Yates et al.  
 2016/0058443 A1 3/2016 Yates et al.  
 2016/0066913 A1 3/2016 Swayze et al.  
 2016/0074040 A1 3/2016 Widenhouse et al.  
 2016/0089137 A1 3/2016 Hess et al.  
 2016/0106431 A1 4/2016 Shelton, IV et al.  
 2016/0113653 A1 4/2016 Zingman  
 2016/0120545 A1 5/2016 Shelton, IV et al.

## FOREIGN PATENT DOCUMENTS

CN 2488482 Y 5/2002  
 CN 1634601 A 7/2005  
 CN 2716900 Y 8/2005  
 CN 2738962 Y 11/2005  
 CN 2868212 Y 2/2007  
 CN 201949071 U 8/2011  
 DE 273689 C 5/1914  
 DE 1775926 A 1/1972  
 DE 3036217 A1 4/1982  
 DE 3210466 A1 9/1983  
 DE 3709067 A1 9/1988  
 DE 19851291 A1 1/2000  
 DE 19924311 A1 11/2000  
 DE 20016423 U1 2/2001  
 DE 20112837 U1 10/2001  
 DE 20121753 U1 4/2003  
 DE 202004012389 U1 9/2004  
 DE 10314072 A1 10/2004  
 DE 202007003114 U1 6/2007  
 EP 0000756 A1 2/1979  
 EP 0122046 A1 10/1984  
 EP 0129442 B1 11/1987  
 EP 0169044 B1 6/1991  
 EP 0548998 A1 6/1993  
 EP 0594148 A1 4/1994  
 EP 0646357 A1 4/1995  
 EP 0505036 B1 5/1995  
 EP 0669104 A1 8/1995  
 EP 0705571 A1 4/1996  
 EP 0770355 A1 5/1997  
 EP 0625335 B1 11/1997  
 EP 0879742 A1 11/1998  
 EP 0650701 B1 3/1999  
 EP 0923907 A1 6/1999  
 EP 0484677 B2 7/2000  
 EP 1034747 A1 9/2000  
 EP 1034748 A1 9/2000  
 EP 1053719 A1 11/2000  
 EP 1055399 A1 11/2000  
 EP 1055400 A1 11/2000  
 EP 1080694 A1 3/2001  
 EP 1090592 A1 4/2001  
 EP 1095627 A1 5/2001  
 EP 0806914 B1 9/2001  
 EP 1284120 A1 2/2003  
 EP 0869742 B1 5/2003  
 EP 1374788 A1 1/2004  
 EP 1407719 A2 4/2004  
 EP 0996378 B1 6/2004  
 EP 1157666 B1 9/2005  
 EP 0880338 B1 10/2005  
 EP 1158917 B1 11/2005  
 EP 1344498 B1 11/2005  
 EP 1330989 B1 12/2005  
 EP 1632191 A2 3/2006  
 EP 1082944 B1 5/2006  
 EP 1253866 B1 7/2006  
 EP 1285633 B1 12/2006  
 EP 1011494 B1 1/2007  
 EP 1767163 A1 3/2007  
 EP 1837041 A1 9/2007  
 EP 0922435 B1 10/2007  
 EP 1599146 B1 10/2007  
 EP 1330201 B1 6/2008  
 EP 2039302 A2 3/2009  
 EP 1719461 B1 6/2009  
 EP 1769754 B1 6/2010  
 EP 1627605 B1 12/2010

(56)

## References Cited

## FOREIGN PATENT DOCUMENTS

EP	2316345	A1	5/2011	JP	2009189838	A	8/2009
EP	2486862	A2	8/2012	JP	2009539420	A	11/2009
EP	2517638	A1	10/2012	JP	2010069310	A	4/2010
EP	2649948	A1	10/2013	JP	2010098844	A	4/2010
EP	2649949	A1	10/2013	KR	20110003229	A	1/2011
EP	2713902	A1	4/2014	RU	2008830	C1	3/1994
FR	459743	A	11/1913	RU	2052979	C1	1/1996
FR	999646	A	2/1952	RU	2098025	C1	12/1997
FR	1112936	A	3/1956	RU	2141279	C1	11/1999
FR	2598905	A1	11/1987	RU	2144791	C1	1/2000
FR	2765794	A1	1/1999	RU	2181566	C2	4/2002
FR	2815842	A1	5/2002	RU	2187249	C2	8/2002
GB	939929	A	10/1963	RU	32984	U1	10/2003
GB	1210522	A	10/1970	RU	2225170	C2	3/2004
GB	1217159	A	12/1970	RU	42750	U1	12/2004
GB	1339394	A	12/1973	RU	61114	U1	2/2007
GB	2024012	A	1/1980	SU	189517	A	1/1967
GB	2109241	A	6/1983	SU	328636	A	9/1972
GB	2272159	A	5/1994	SU	674747	A1	7/1979
GB	2336214	A	10/1999	SU	1009439	A	4/1983
GR	930100110	A	11/1993	SU	1333319	A2	8/1987
JP	S4711908	Y1	5/1972	SU	1377053	A1	2/1988
JP	S5033988	U	4/1975	SU	1509051	A1	9/1989
JP	S56112235	A	9/1981	SU	1561964	A1	5/1990
JP	S62170011	U	10/1987	SU	1708312	A1	1/1992
JP	H04215747	A	8/1992	SU	1722476	A1	3/1992
JP	H04131860	U	12/1992	SU	1752361	A1	8/1992
JP	H0584252	A	4/1993	SU	1814161	A1	5/1993
JP	H05123325	A	5/1993	WO	WO-9315648	A1	8/1993
JP	H0630945	A	2/1994	WO	WO-9420030	A1	9/1994
JP	H06237937	A	8/1994	WO	WO-9517855	A1	7/1995
JP	H06327684	A	11/1994	WO	WO-9520360	A1	8/1995
JP	H07124166	A	5/1995	WO	WO-9623448	A1	8/1996
JP	H07255735	A	10/1995	WO	WO-9635464	A1	11/1996
JP	H07285089	A	10/1995	WO	WO-9639086	A1	12/1996
JP	H0833642	A	2/1996	WO	WO-9639088	A1	12/1996
JP	H08164141	A	6/1996	WO	WO-9724073	A1	7/1997
JP	H08182684	A	7/1996	WO	WO-9734533	A1	9/1997
JP	H08507708	A	8/1996	WO	WO-9903407	A1	1/1999
JP	H08229050	A	9/1996	WO	WO-9903409	A1	1/1999
JP	H10118090	A	5/1998	WO	WO-9948430	A1	9/1999
JP	2000014632	A	1/2000	WO	WO-0024322	A1	5/2000
JP	2000033071	A	2/2000	WO	WO-0024330	A1	5/2000
JP	2000112002	A	4/2000	WO	WO-0053112	A2	9/2000
JP	2000166932	A	6/2000	WO	WO-0057796	A1	10/2000
JP	2000171730	A	6/2000	WO	WO-0105702	A1	1/2001
JP	2000287987	A	10/2000	WO	WO-0154594	A1	8/2001
JP	2000325303	A	11/2000	WO	WO-0158371	A1	8/2001
JP	2001087272	A	4/2001	WO	WO-0162164	A2	8/2001
JP	2001514541	A	9/2001	WO	WO-0162169	A2	8/2001
JP	2001276091	A	10/2001	WO	WO-0191646	A1	12/2001
JP	2002051974	A	2/2002	WO	WO-0219932	A1	3/2002
JP	2002085415	A	3/2002	WO	WO-0226143	A1	4/2002
JP	2002143078	A	5/2002	WO	WO-0236028	A1	5/2002
JP	2002528161	A	9/2002	WO	WO-02065933	A2	8/2002
JP	2002314298	A	10/2002	WO	WO-03055402	A1	7/2003
JP	2003135473	A	5/2003	WO	WO-03094747	A1	11/2003
JP	2003521301	A	7/2003	WO	WO-03079909	A3	3/2004
JP	2004147701	A	5/2004	WO	WO-2004019803	A1	3/2004
JP	2004162035	A	6/2004	WO	WO-2004032783	A1	4/2004
JP	2004229976	A	8/2004	WO	WO-2004047626	A1	6/2004
JP	2005080702	A	3/2005	WO	WO-2004047653	A2	6/2004
JP	2005131163	A	5/2005	WO	WO-2004056277	A1	7/2004
JP	2005131164	A	5/2005	WO	WO-2004078050	A2	9/2004
JP	2005131173	A	5/2005	WO	WO-2004078051	A2	9/2004
JP	2005131211	A	5/2005	WO	WO-2004096015	A2	11/2004
JP	2005131212	A	5/2005	WO	WO-2006044581	A2	4/2006
JP	2005137423	A	6/2005	WO	WO-2006051252	A1	5/2006
JP	2005328882	A	12/2005	WO	WO-2006059067	A1	6/2006
JP	2005335432	A	12/2005	WO	WO-2006085389	A1	8/2006
JP	2005342267	A	12/2005	WO	WO-2007074430	A1	7/2007
JP	2006187649	A	7/2006	WO	WO-2007129121	A1	11/2007
JP	2006281405	A	10/2006	WO	WO-2007137304	A2	11/2007
JP	2006346445	A	12/2006	WO	WO-2007142625	A2	12/2007
JP	2009507526	A	2/2009	WO	WO-2008021969	A2	2/2008
				WO	WO-2008089404	A2	7/2008
				WO	WO-2009005969	A2	1/2009
				WO	WO-2009067649	A2	5/2009
				WO	WO-2009091497	A2	7/2009

(56)

**References Cited**

## FOREIGN PATENT DOCUMENTS

WO WO-2011008672 A2 1/2011  
 WO WO-2011044343 A2 4/2011  
 WO WO-2012006306 A2 1/2012  
 WO WO-2012044606 A2 4/2012

## OTHER PUBLICATIONS

Fast, Versatile Blackfin Processors Handle Advanced RFID Reader Applications; Analog Dialogue: vol. 40—Sep. 2006; <http://www.analog.com/library/analogDialogue/archives/40-09/rfid.pdf>; Wayback Machine to Feb. 15, 2012.

Covidien Brochure, “Endo GIA™ Black Reload with Tri-Staple™ Technology,” (2012), 2 pages.

The Sodem Aseptic Battery Transfer Kit, Sodem Systems, 2000, 3 pages.

Schellhammer et al., “Poly-Lactic-Acid for Coating of Endovascular Stents: Preliminary Results in Canine Experimental Av-Fistulae,” *Mat.-wiss. u. Werkstofftech.*, 32, pp. 193-199 (2001).

Miyata et al., “Biomolecule-Sensitive Hydrogels,” *Advanced Drug Delivery Reviews*, 54 (2002) pp. 79-98.

Jeong et al., “Thermosensitive Sol-Gel Reversible Hydrogels,” *Advanced Drug Delivery Reviews*, 54 (2002) pp. 37-51.

Covidien Brochure, “Endo GIA™ Ultra Universal Stapler,” (2010), 2 pages.

Qiu et al., “Environment-Sensitive Hydrogels for Drug Delivery,” *Advanced Drug Delivery Reviews*, 53 (2001) pp. 321-339.

Hoffman, “Hydrogels for Biomedical Applications,” *Advanced Drug Delivery Reviews*, 43 (2002) pp. 3-12.

Hoffman, “Hydrogels for Biomedical Applications,” *Advanced Drug Delivery Reviews*, 54 (2002) pp. 3-12.

Peppas, “Physiologically Responsive Hydrogels,” *Journal of Bioactive and Compatible Polymers*, vol. 6 (Jul. 1991) pp. 241-246.

Peppas, Editor “Hydrogels in Medicine and Pharmacy,” vol. I, Fundamentals, CRC Press, 1986.

Young, “Microcellular foams via phase separation,” *Journal of Vacuum Science & Technology A* 4(3), (May/Jun. 1986).

Chen et al., “Elastomeric Biomaterials for Tissue Engineering,” *Progress in Polymer Science* 38 (2013), pp. 584-671.

Ebara, “Carbohydrate-Derived Hydrogels and Microgels,” *Engineered Carbohydrate-Based Materials for Biomedical Applications: Polymers, Surfaces, Dendrimers, Nanoparticles, and Hydrogels*, Edited by Ravin Narain, 2011, pp. 337-345.

Matsuda, “Thermodynamics of Formation of Porous Polymeric Membrane from Solutions,” *Polymer Journal*, vol. 23, No. 5, pp. 435-444 (1991).

Byrne et al., “Molecular Imprinting Within Hydrogels,” *Advanced Drug Delivery Reviews*, 54 (2002) pp. 149-161.

Covidien Brochure, “Endo GIA™ Reloads with Tri-Staple™ Technology,” (2010), 1 page.

Covidien Brochure, “Endo GIA™ Reloads with Tri-Staple™ Technology and Endo GIA™ Ultra Universal Staplers,” (2010), 2 pages.

Covidien Brochure, “Endo GIA™ Curved Tip Reload with Tri-Staple™ Technology,” (2012), 2 pages.

Covidien Brochure, “Endo GIA™ Reloads with Tri-Staple™ Technology,” (2010), 2 pages.

<http://ninpgan.net/publications/51-100/89.pdf>; 2004, Ning Pan, on Uniqueness of Fibrous Materials, *Design & Nature II*. Eds: Colins, M. and Brebbia, C. WIT Press, Boston, 493-504.

D. Tuite, Ed., “Get the Lowdown on Ultracapacitors,” Nov. 15, 2007; [online] URL: <http://electronicdesign.com/Articles/Print.cfm?ArticleID=17465>, accessed Jan. 15, 2008 (5 pages).

C.C. Thompson et al., “Peroral Endoscopic Reduction of Dilated Gastrojejunal Anastomosis After Roux-en-Y Gastric Bypass: A Possible New Option for Patients with Weight Regain,” *Surg Endosc* (2006) vol. 20., pp. 1744-1748.

Datasheet for Panasonic TK Relays Ultra Low Profile 2 A Polarized Relay, Copyright Matsushita Electric Works, Ltd. (Known of at least as early as Aug. 17, 2010), 5 pages.

B.R. Coolman, DVM, MS et al., “Comparison of Skin Staples With Sutures for Anastomosis of the Small Intestine in Dogs,” Abstract; <http://www.blackwell-synergy.com/doi/abs/10.1053/jvet.2000.7539?cookieSet=1&journalCode=vsu> which redirects to <http://www3.interscience.wiley.com/journal/119040681/abstract?CRETRY=1&SRETRY=0>; [online] accessed: Sep. 22, 2008 (2 pages).

Indian Standard: Automotive Vehicles—Brakes and Braking Systems (IS 11852-1:2001), Mar. 1, 2001.

Disclosed Anonymously, “Motor-Driven Surgical Stapler Improvements,” Research Disclosure Database No. 526041, Published: Feb. 2008.

Van Meer et al., “A Disposable Plastic Compact Wrist for Smart Minimally Invasive Surgical Tools,” LAAS/CNRS (Aug. 2005).

Breedveld et al., “A New, Easily Miniaturized Sterrable Endoscope,” *IEEE Engineering in Medicine and Biology Magazine* (Nov./Dec. 2005).

ASTM procedure D2240-00, “Standard Test Method for Rubber Property-Durometer Hardness,” (Published Aug. 2000).

ASTM procedure D2240-05, “Standard Test Method for Rubber Property-Durometer Hardness,” (Published Apr. 2010).

Pitt et al., “Attachment of Hyaluronan to Metallic Surfaces,” *J. Biomed. Mater. Res.* 68A: pp. 95-106, 2004.

Solorio et al., “Gelatin Microspheres Crosslinked with Genipin for Local Delivery of Growth Factors,” *J. Tissue Eng. Regen. Med.* (2010), 4(7): pp. 514-523.

Covidien iDrive™ Ultra in Service Reference Card, “iDrive™ Ultra Powered Stapling Device,” (4 pages).

Covidien iDrive™ Ultra Powered Stapling System brochure, “The Power of iDrive™ Ultra Powered Stapling System and Tri-Staple™ Technology,” (23 pages).

Covidien “iDrive™ Ultra Powered Stapling System, A Guide for Surgeons,” (6 pages).

Covidien “iDrive™ Ultra Powered Stapling System, Cleaning and Sterilization Guide,” (2 pages).

Covidien Brochure “iDrive™ Ultra Powered Stapling System,” (6 pages).

Seils et al., Covidien Summary: Clinical Study “UCONN Biodynamics: Final Report on Results,” (2 pages).

Biomedical Coatings, Fort Wayne Metals, Research Products Corporation, obtained online at [www.fwmetals.com](http://www.fwmetals.com) on Jun. 21, 2010 (1 page).

\* cited by examiner



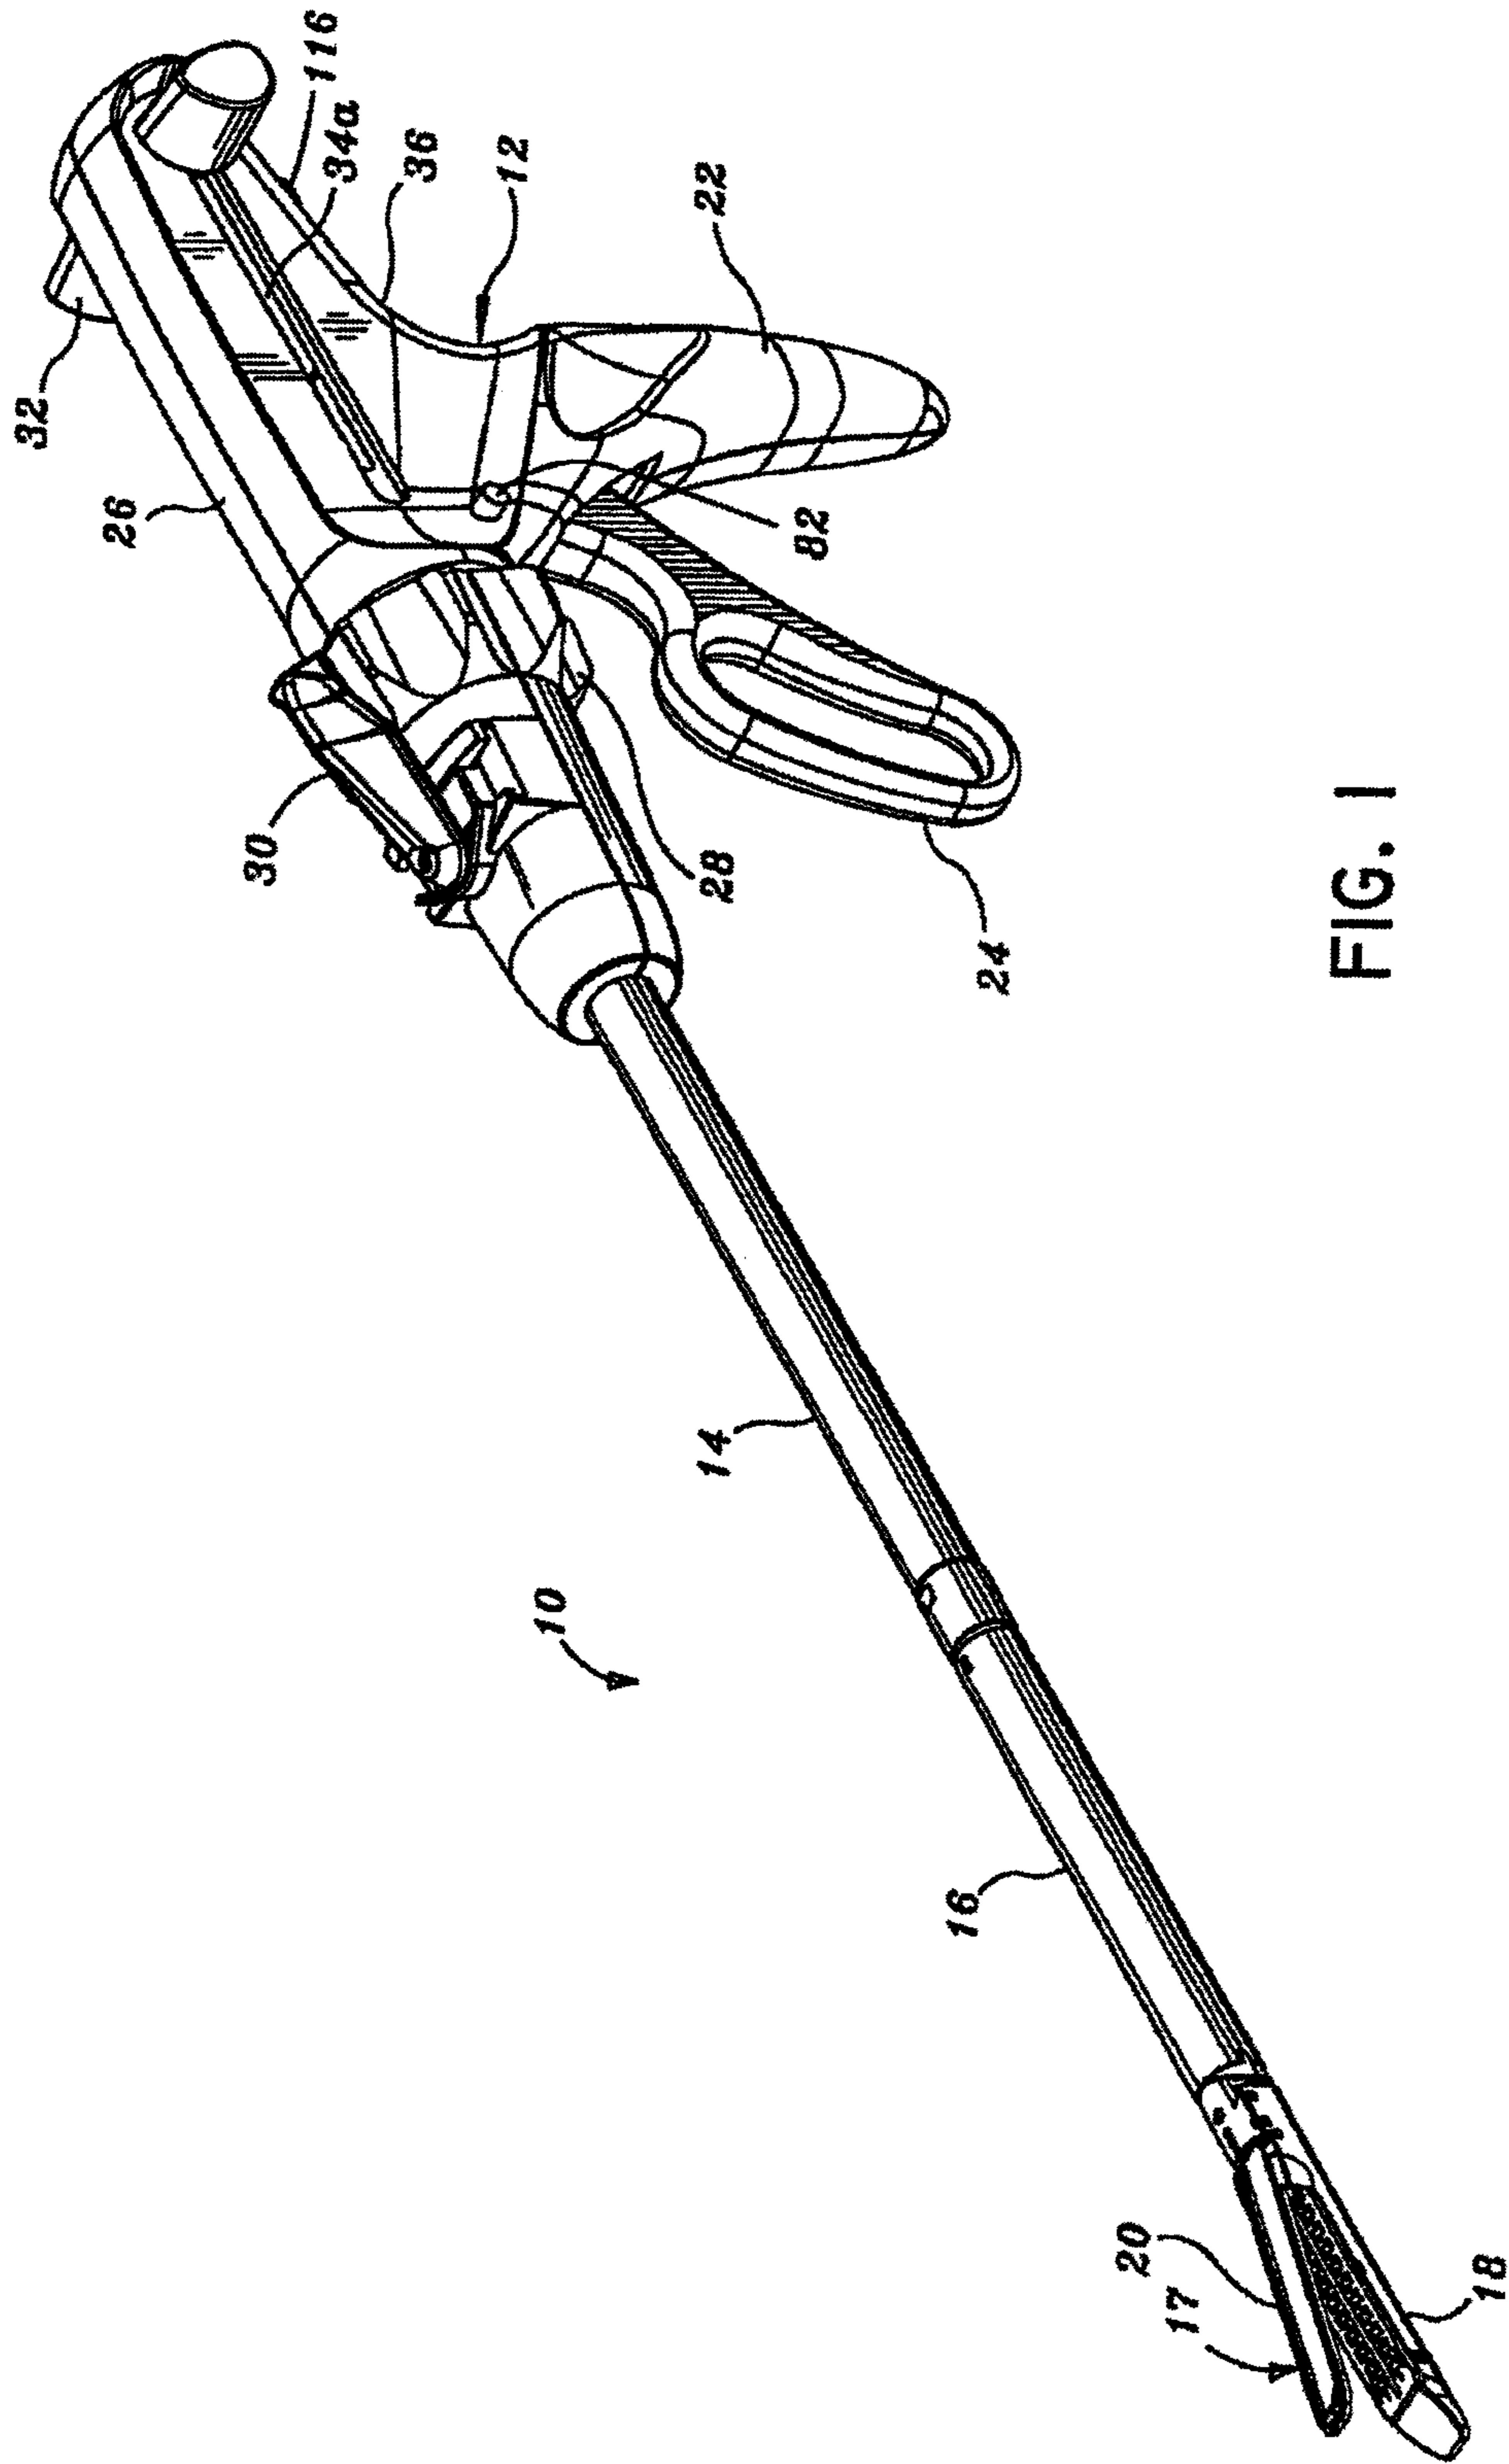


FIG. 1



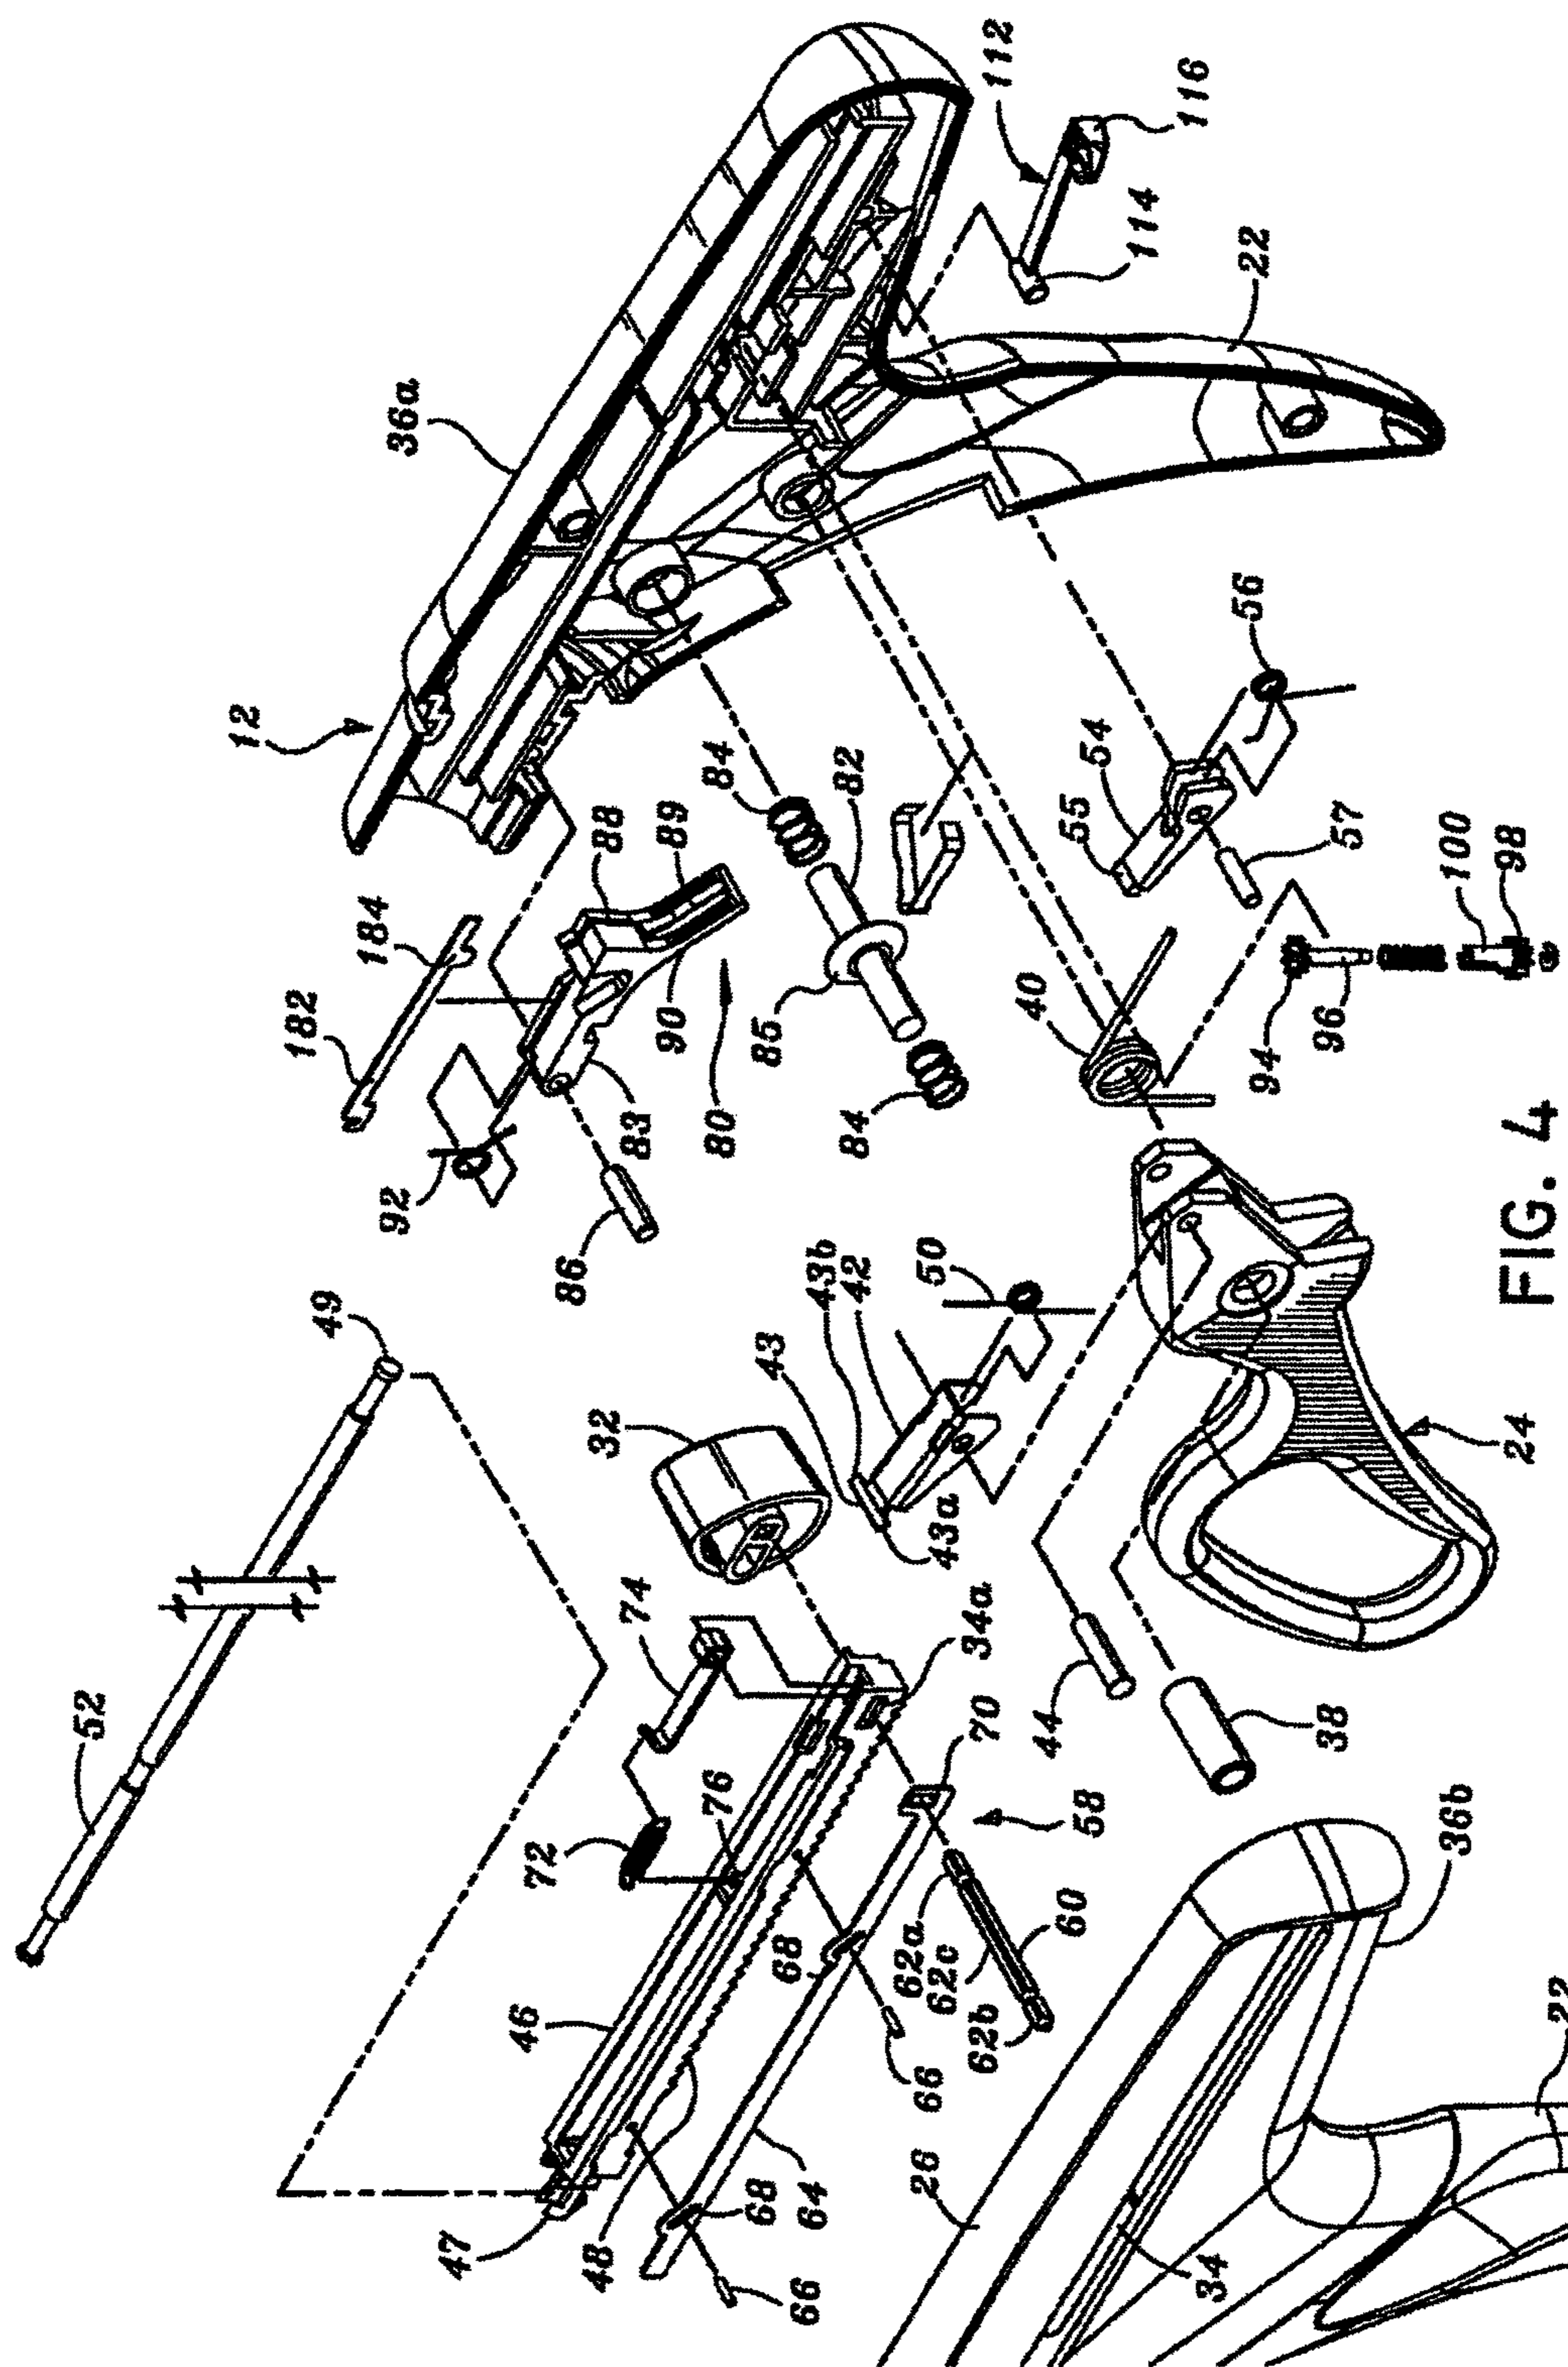
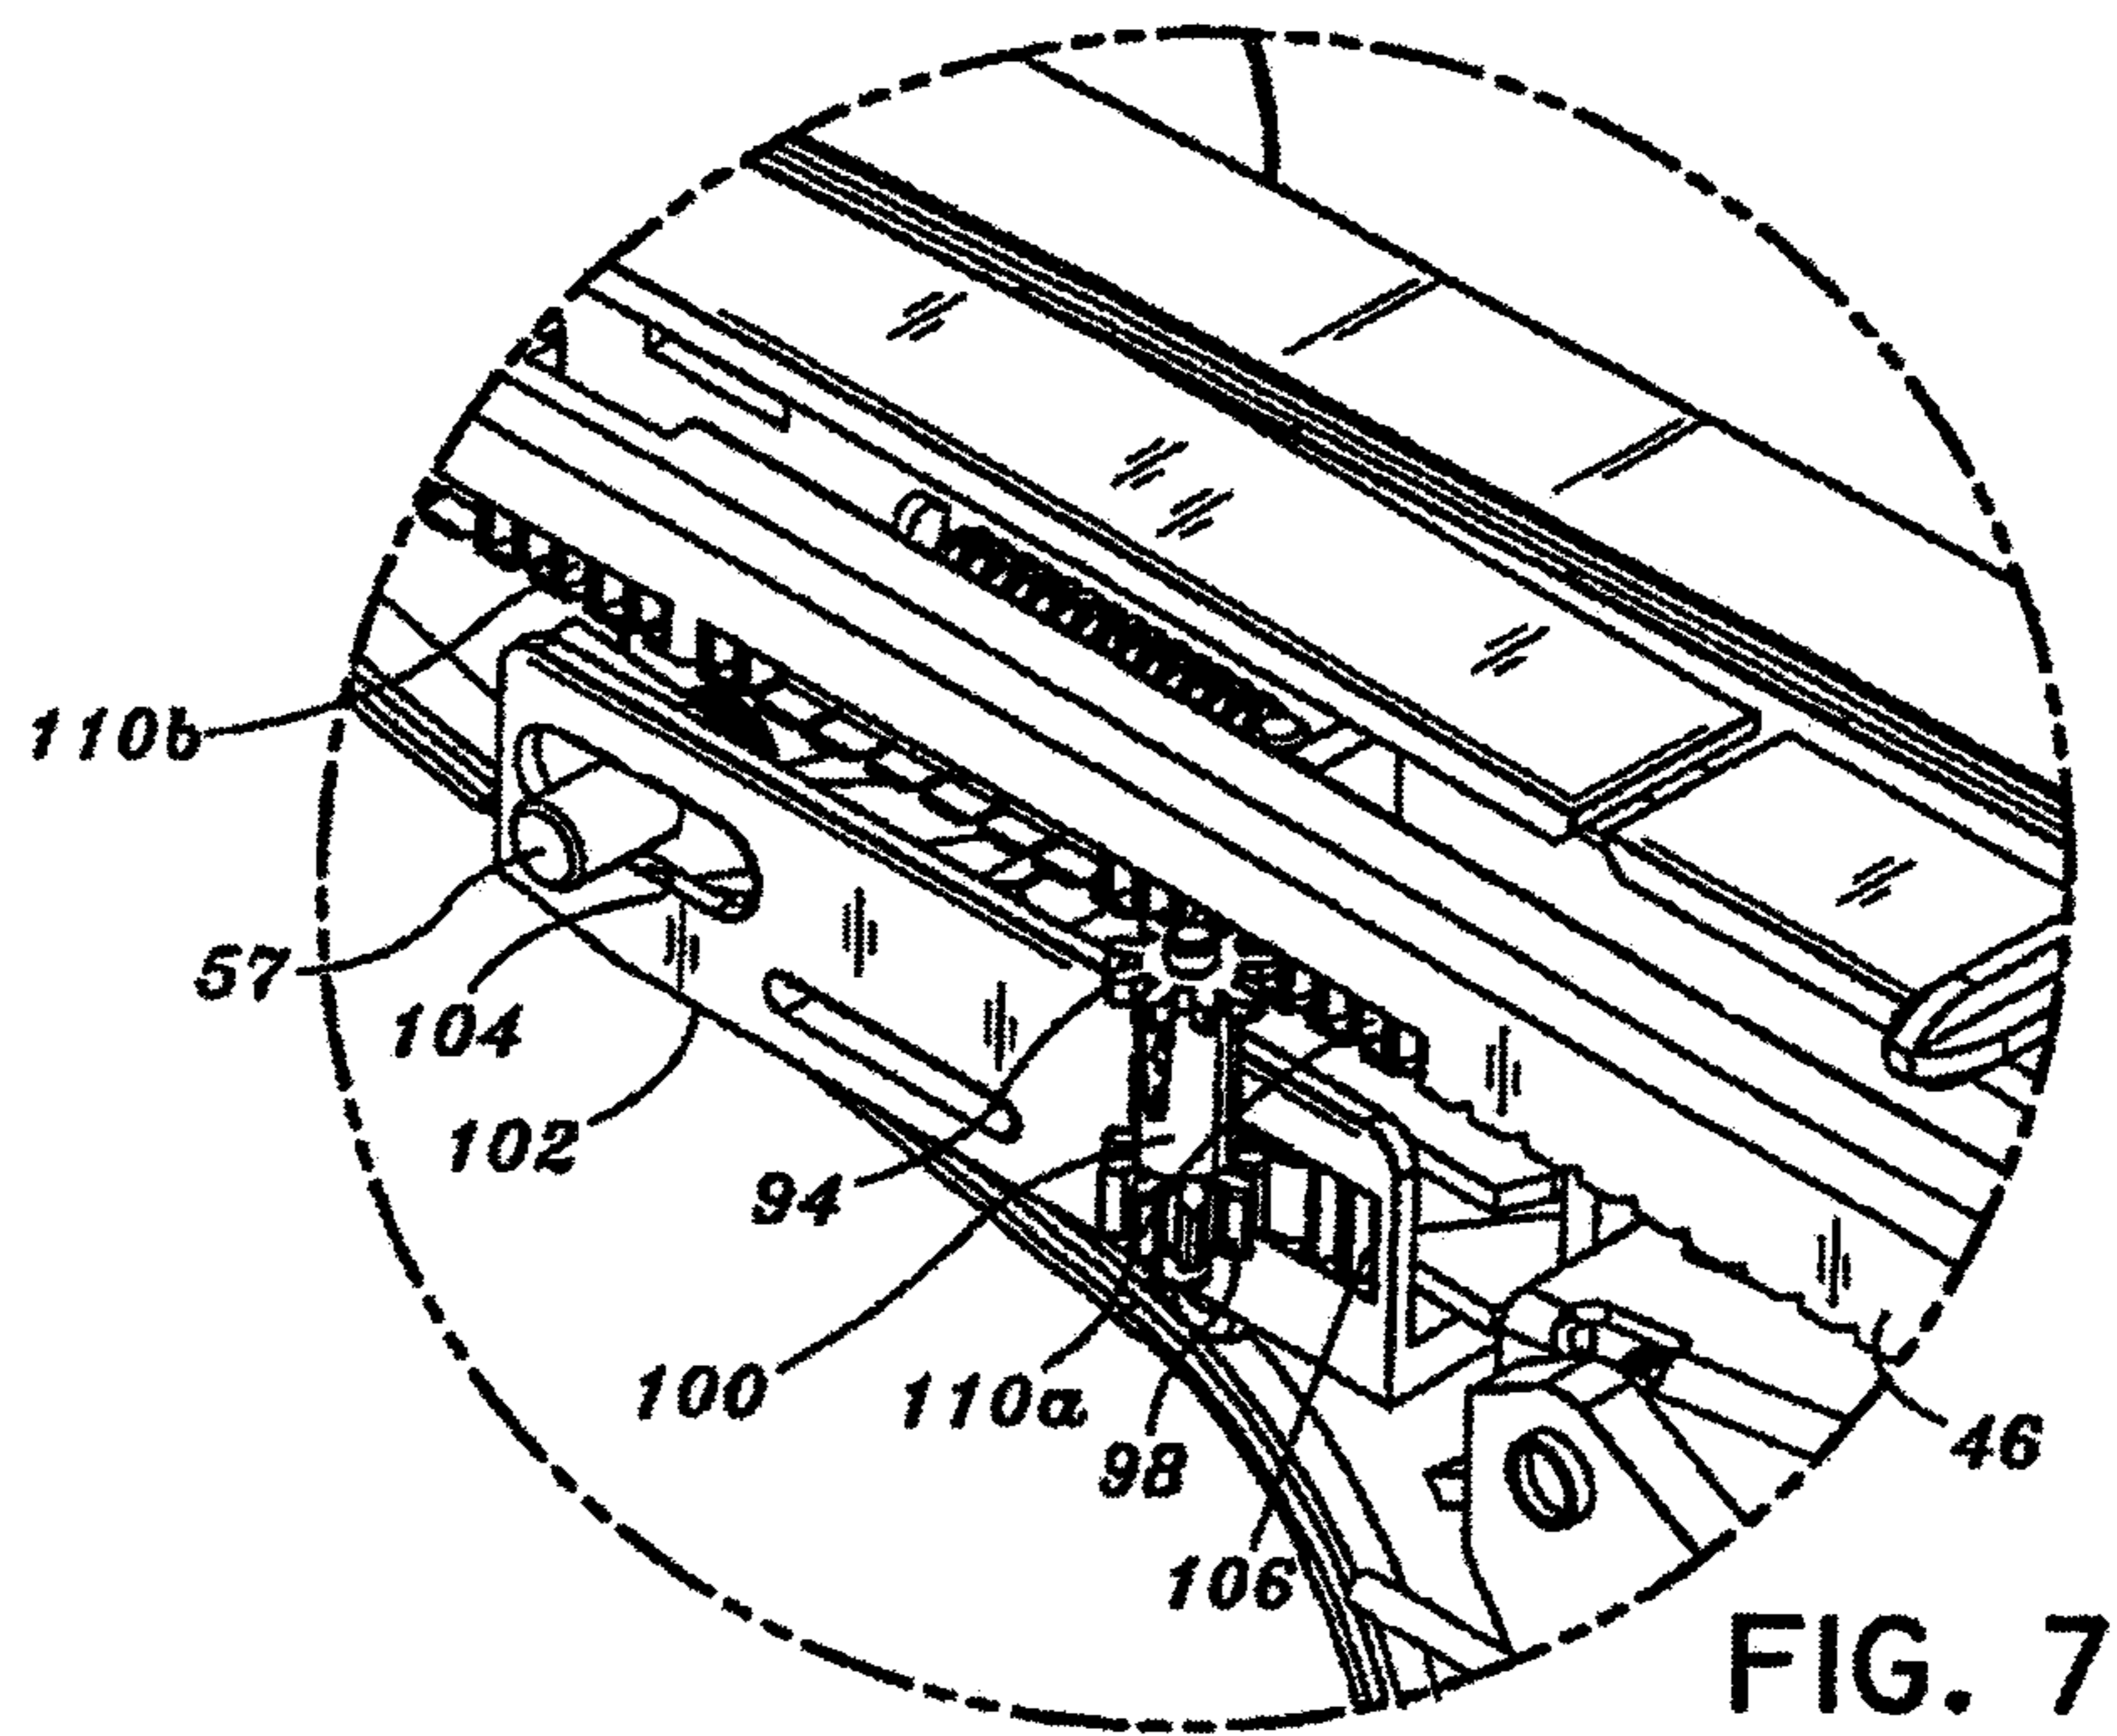
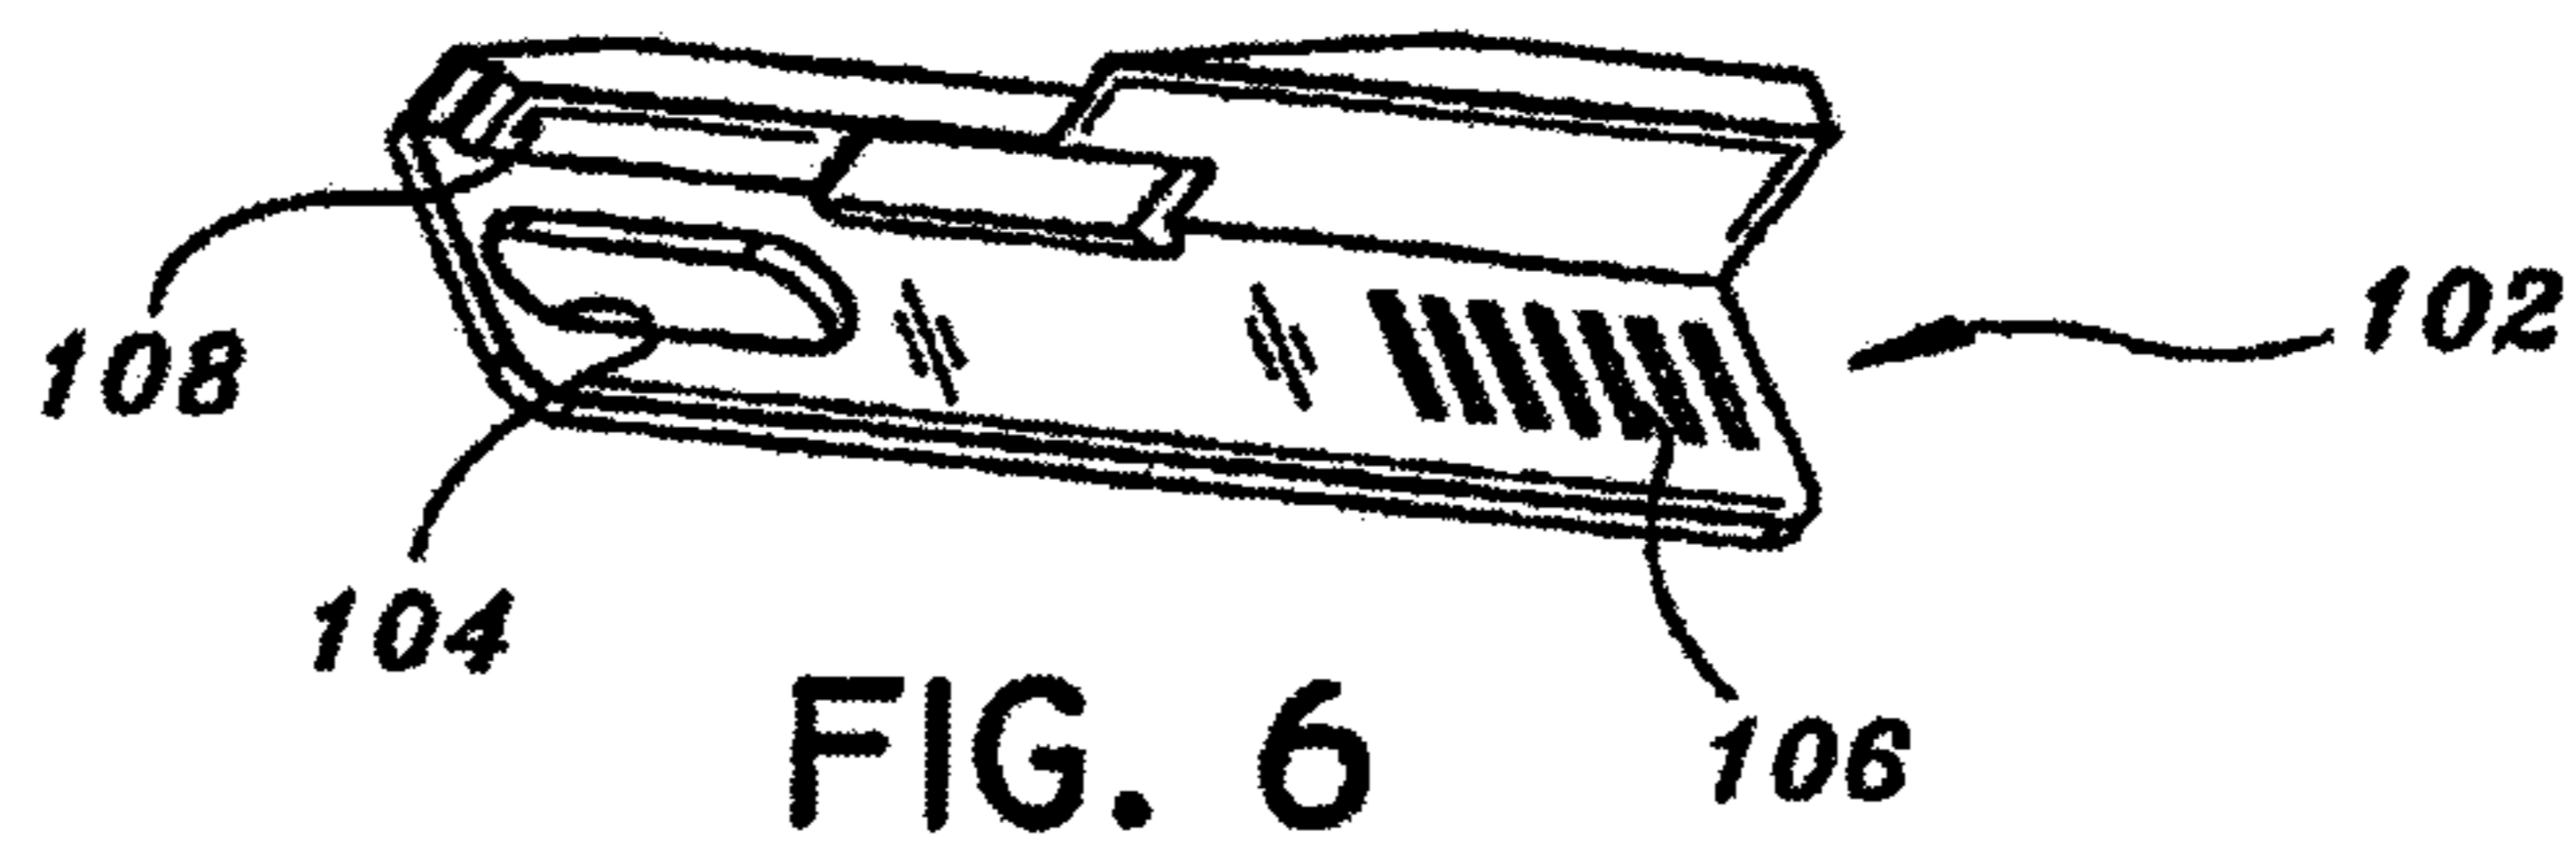
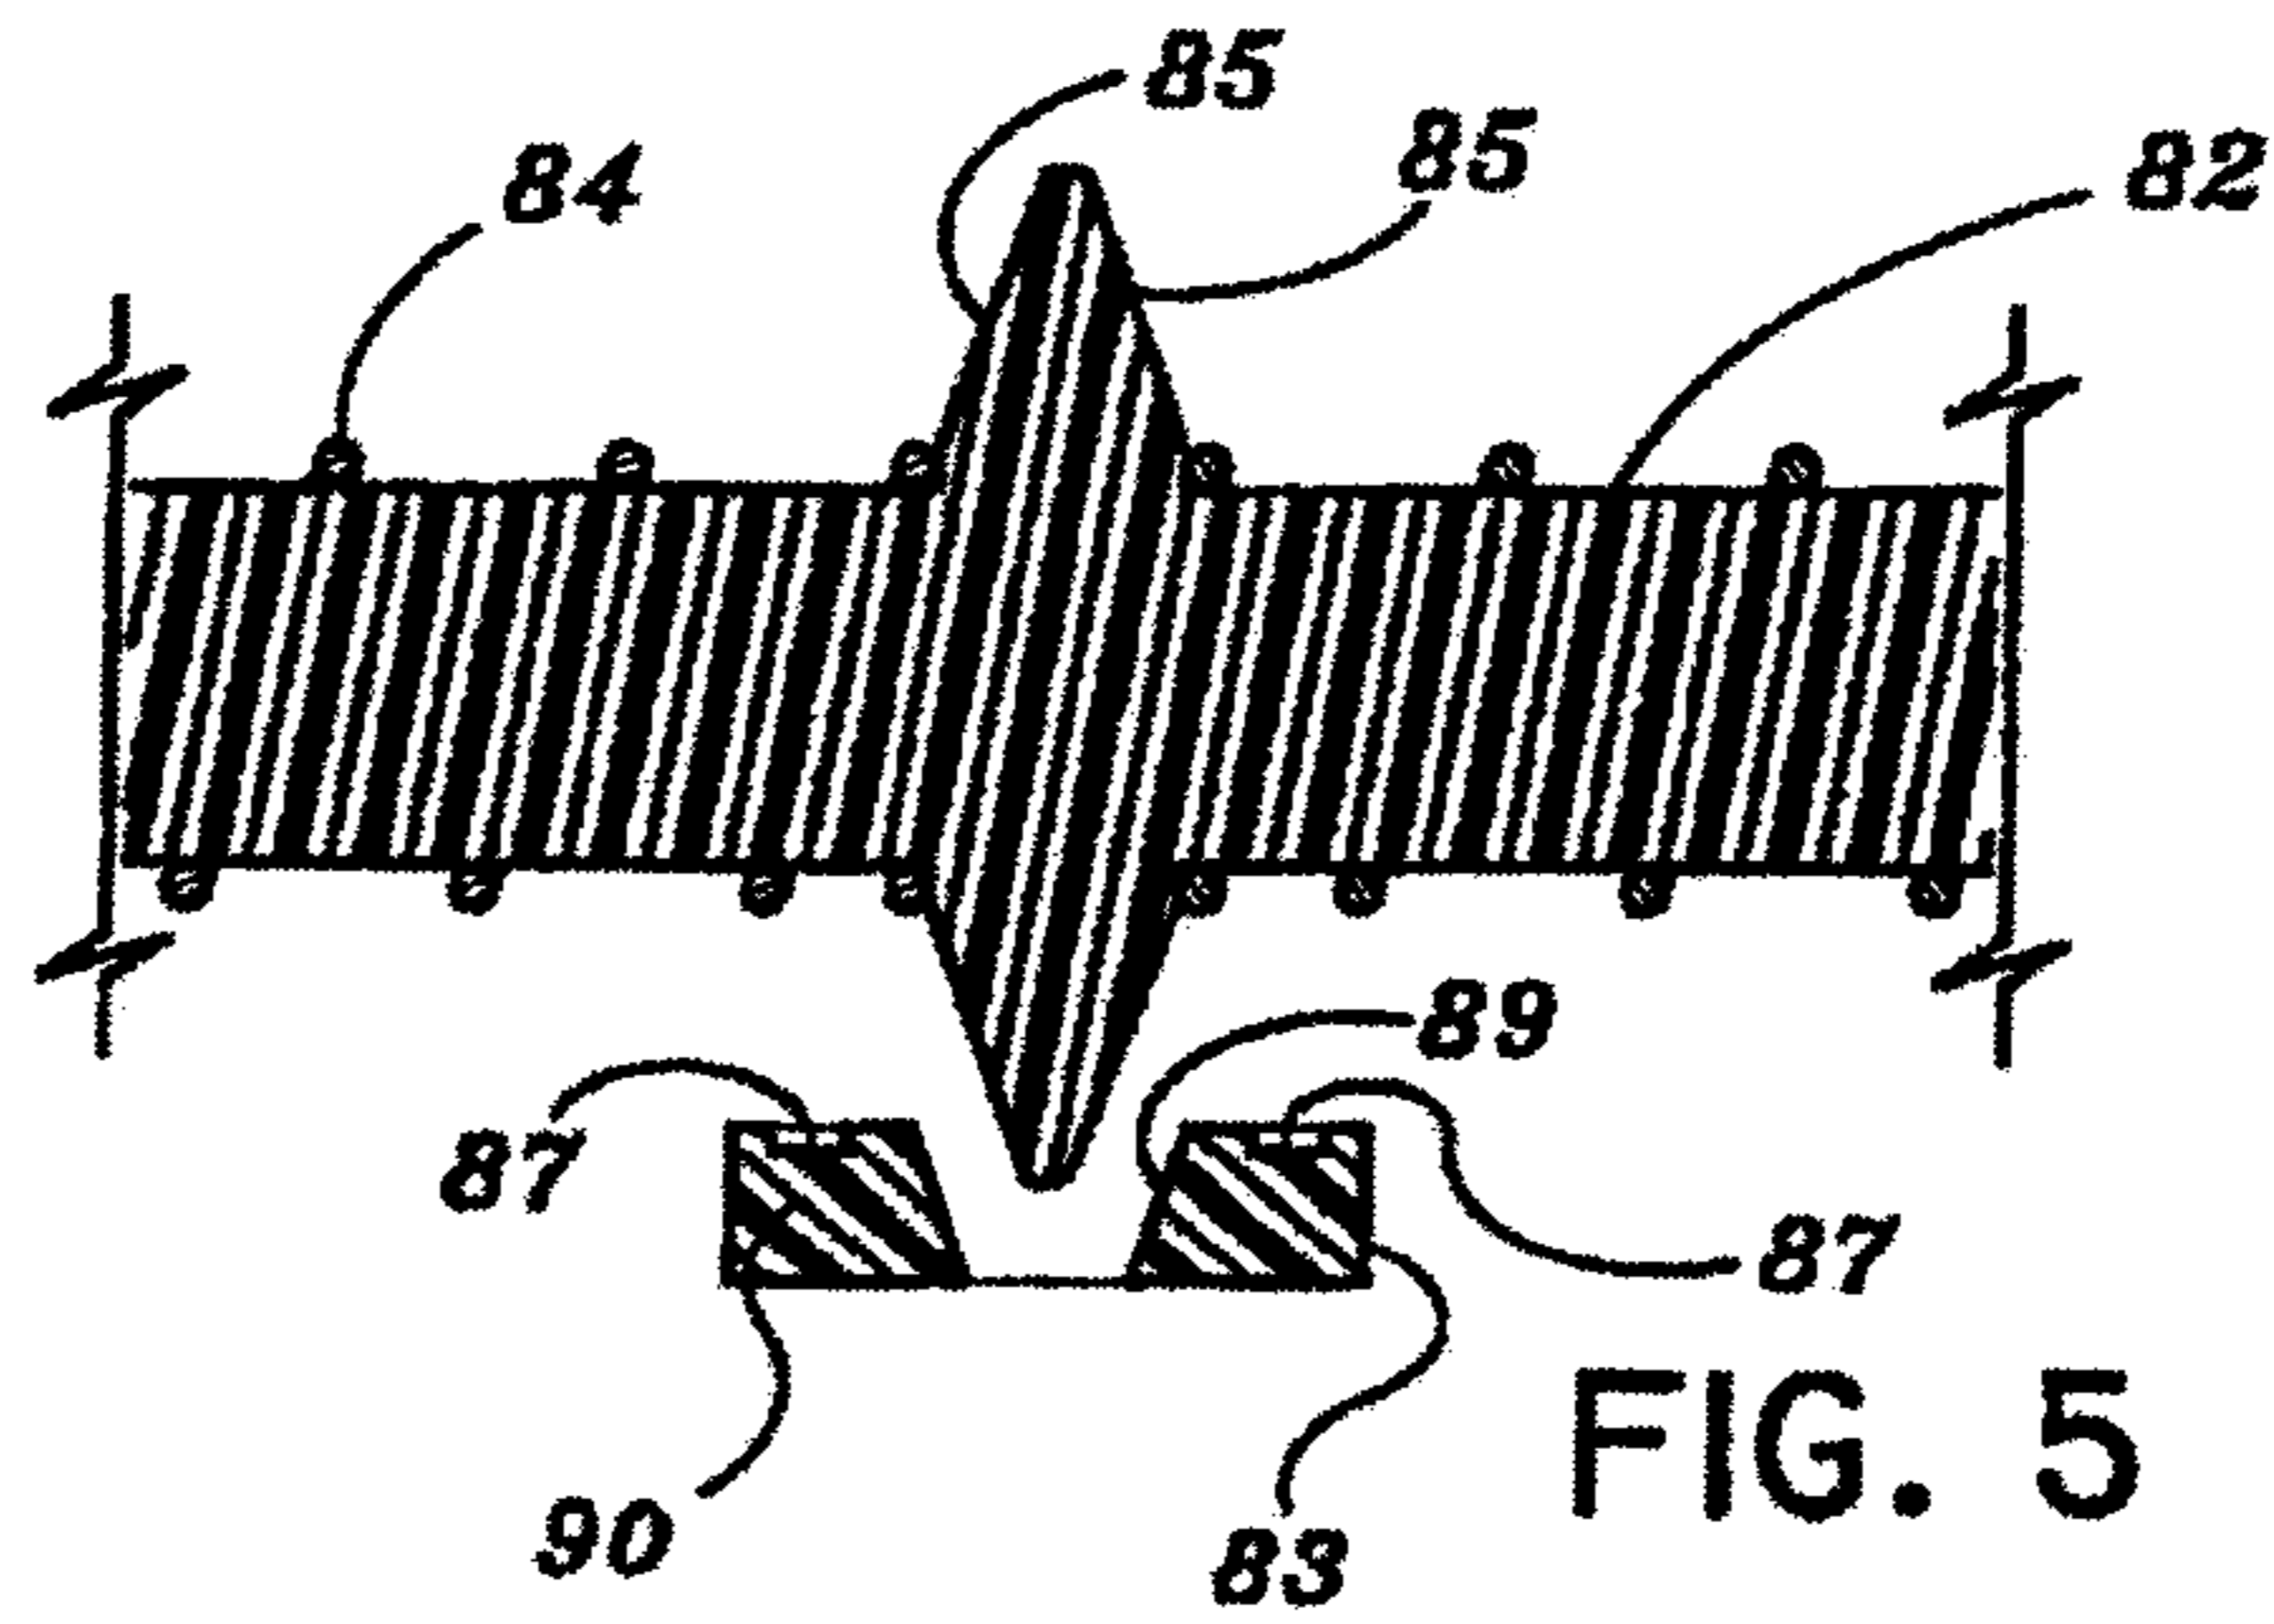
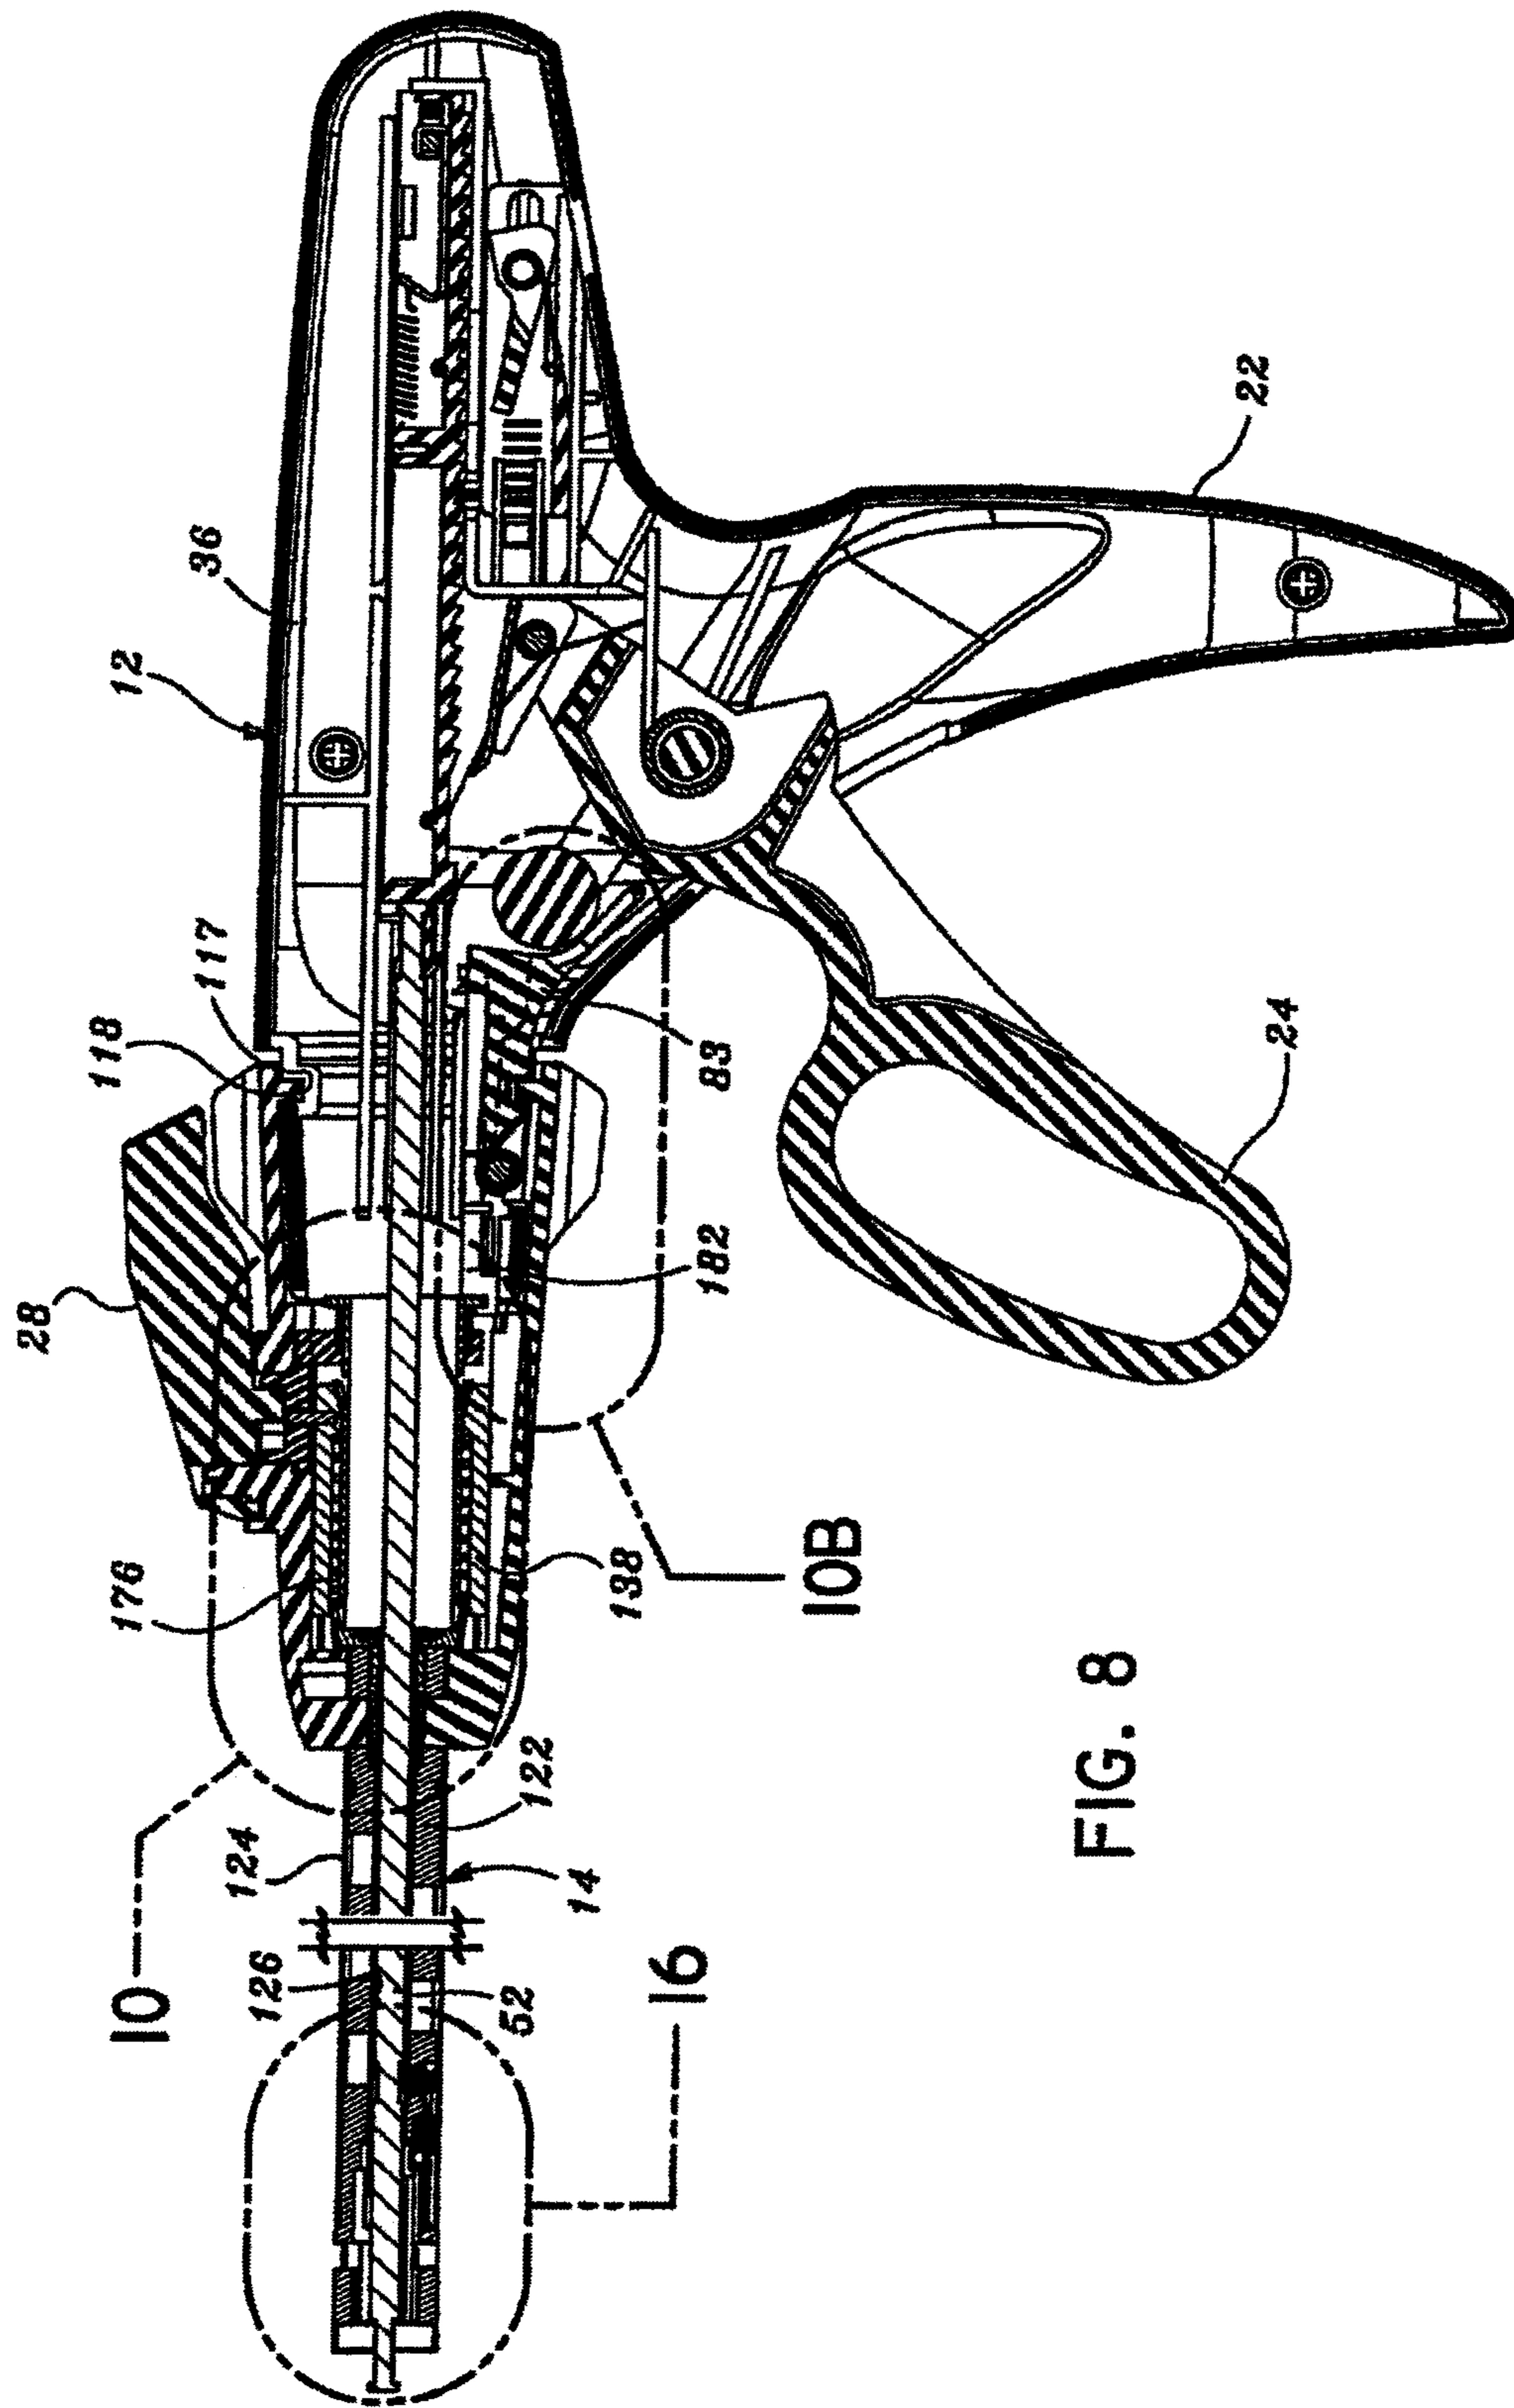


FIG. 4





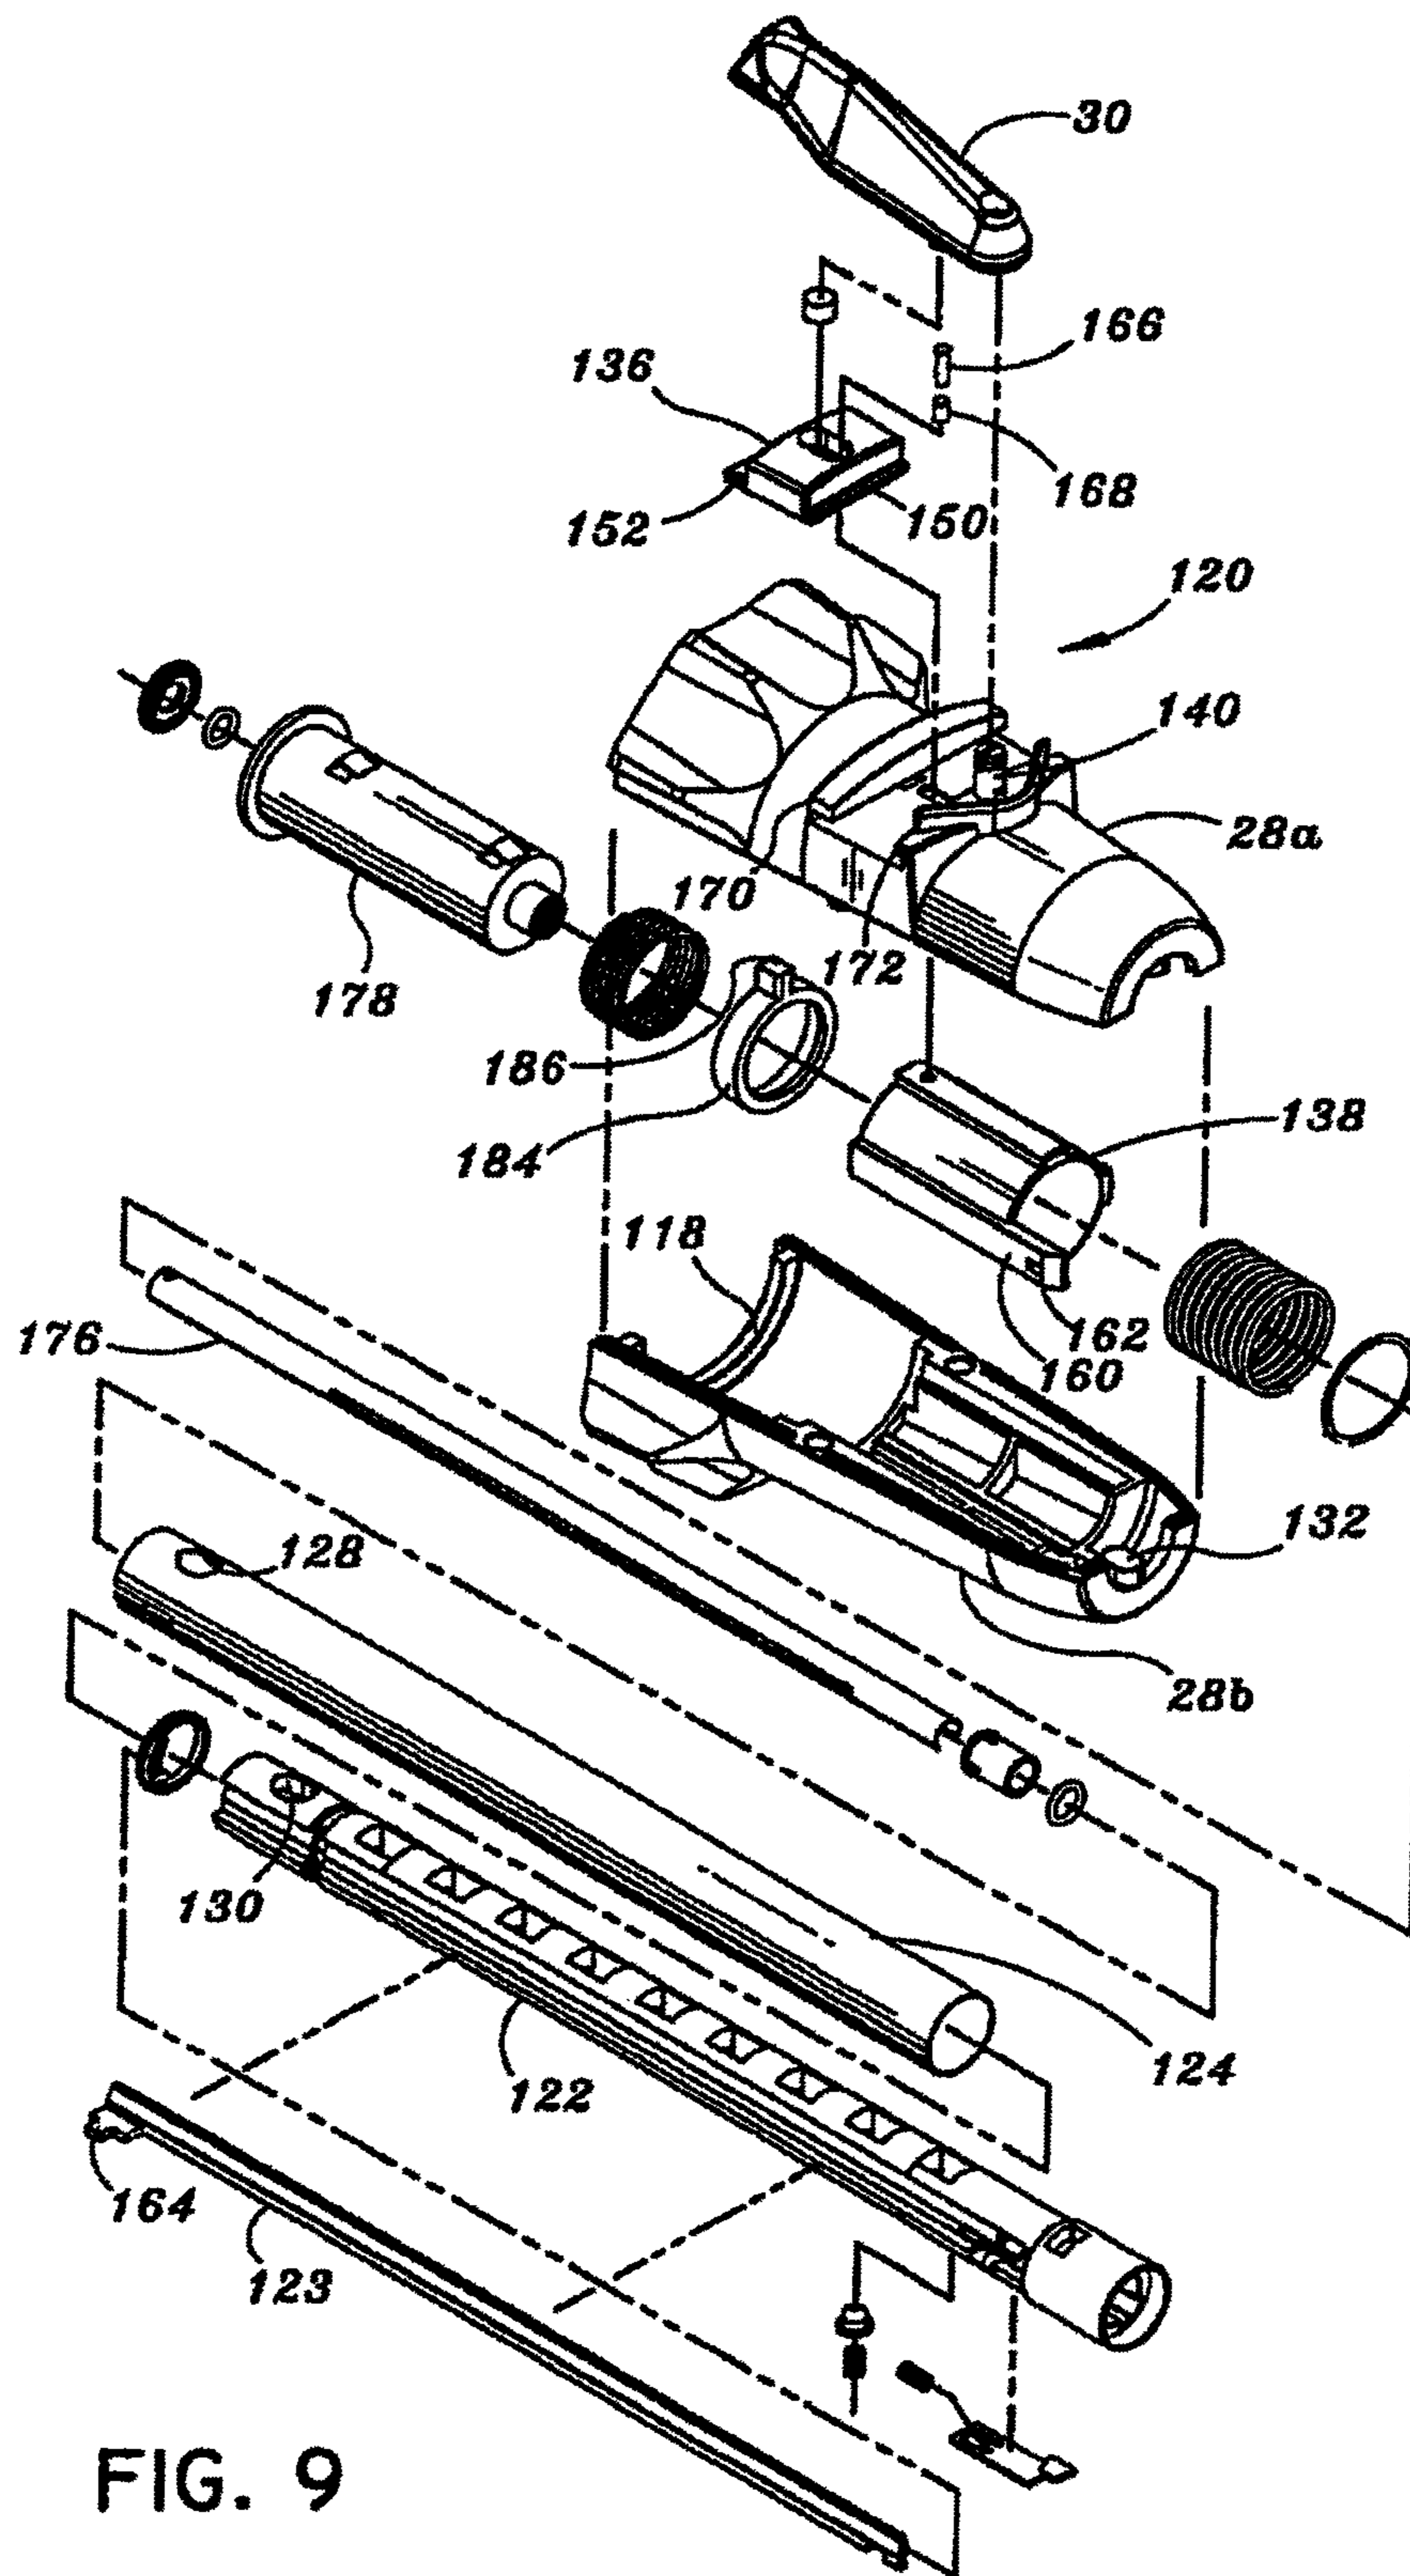


FIG. 9

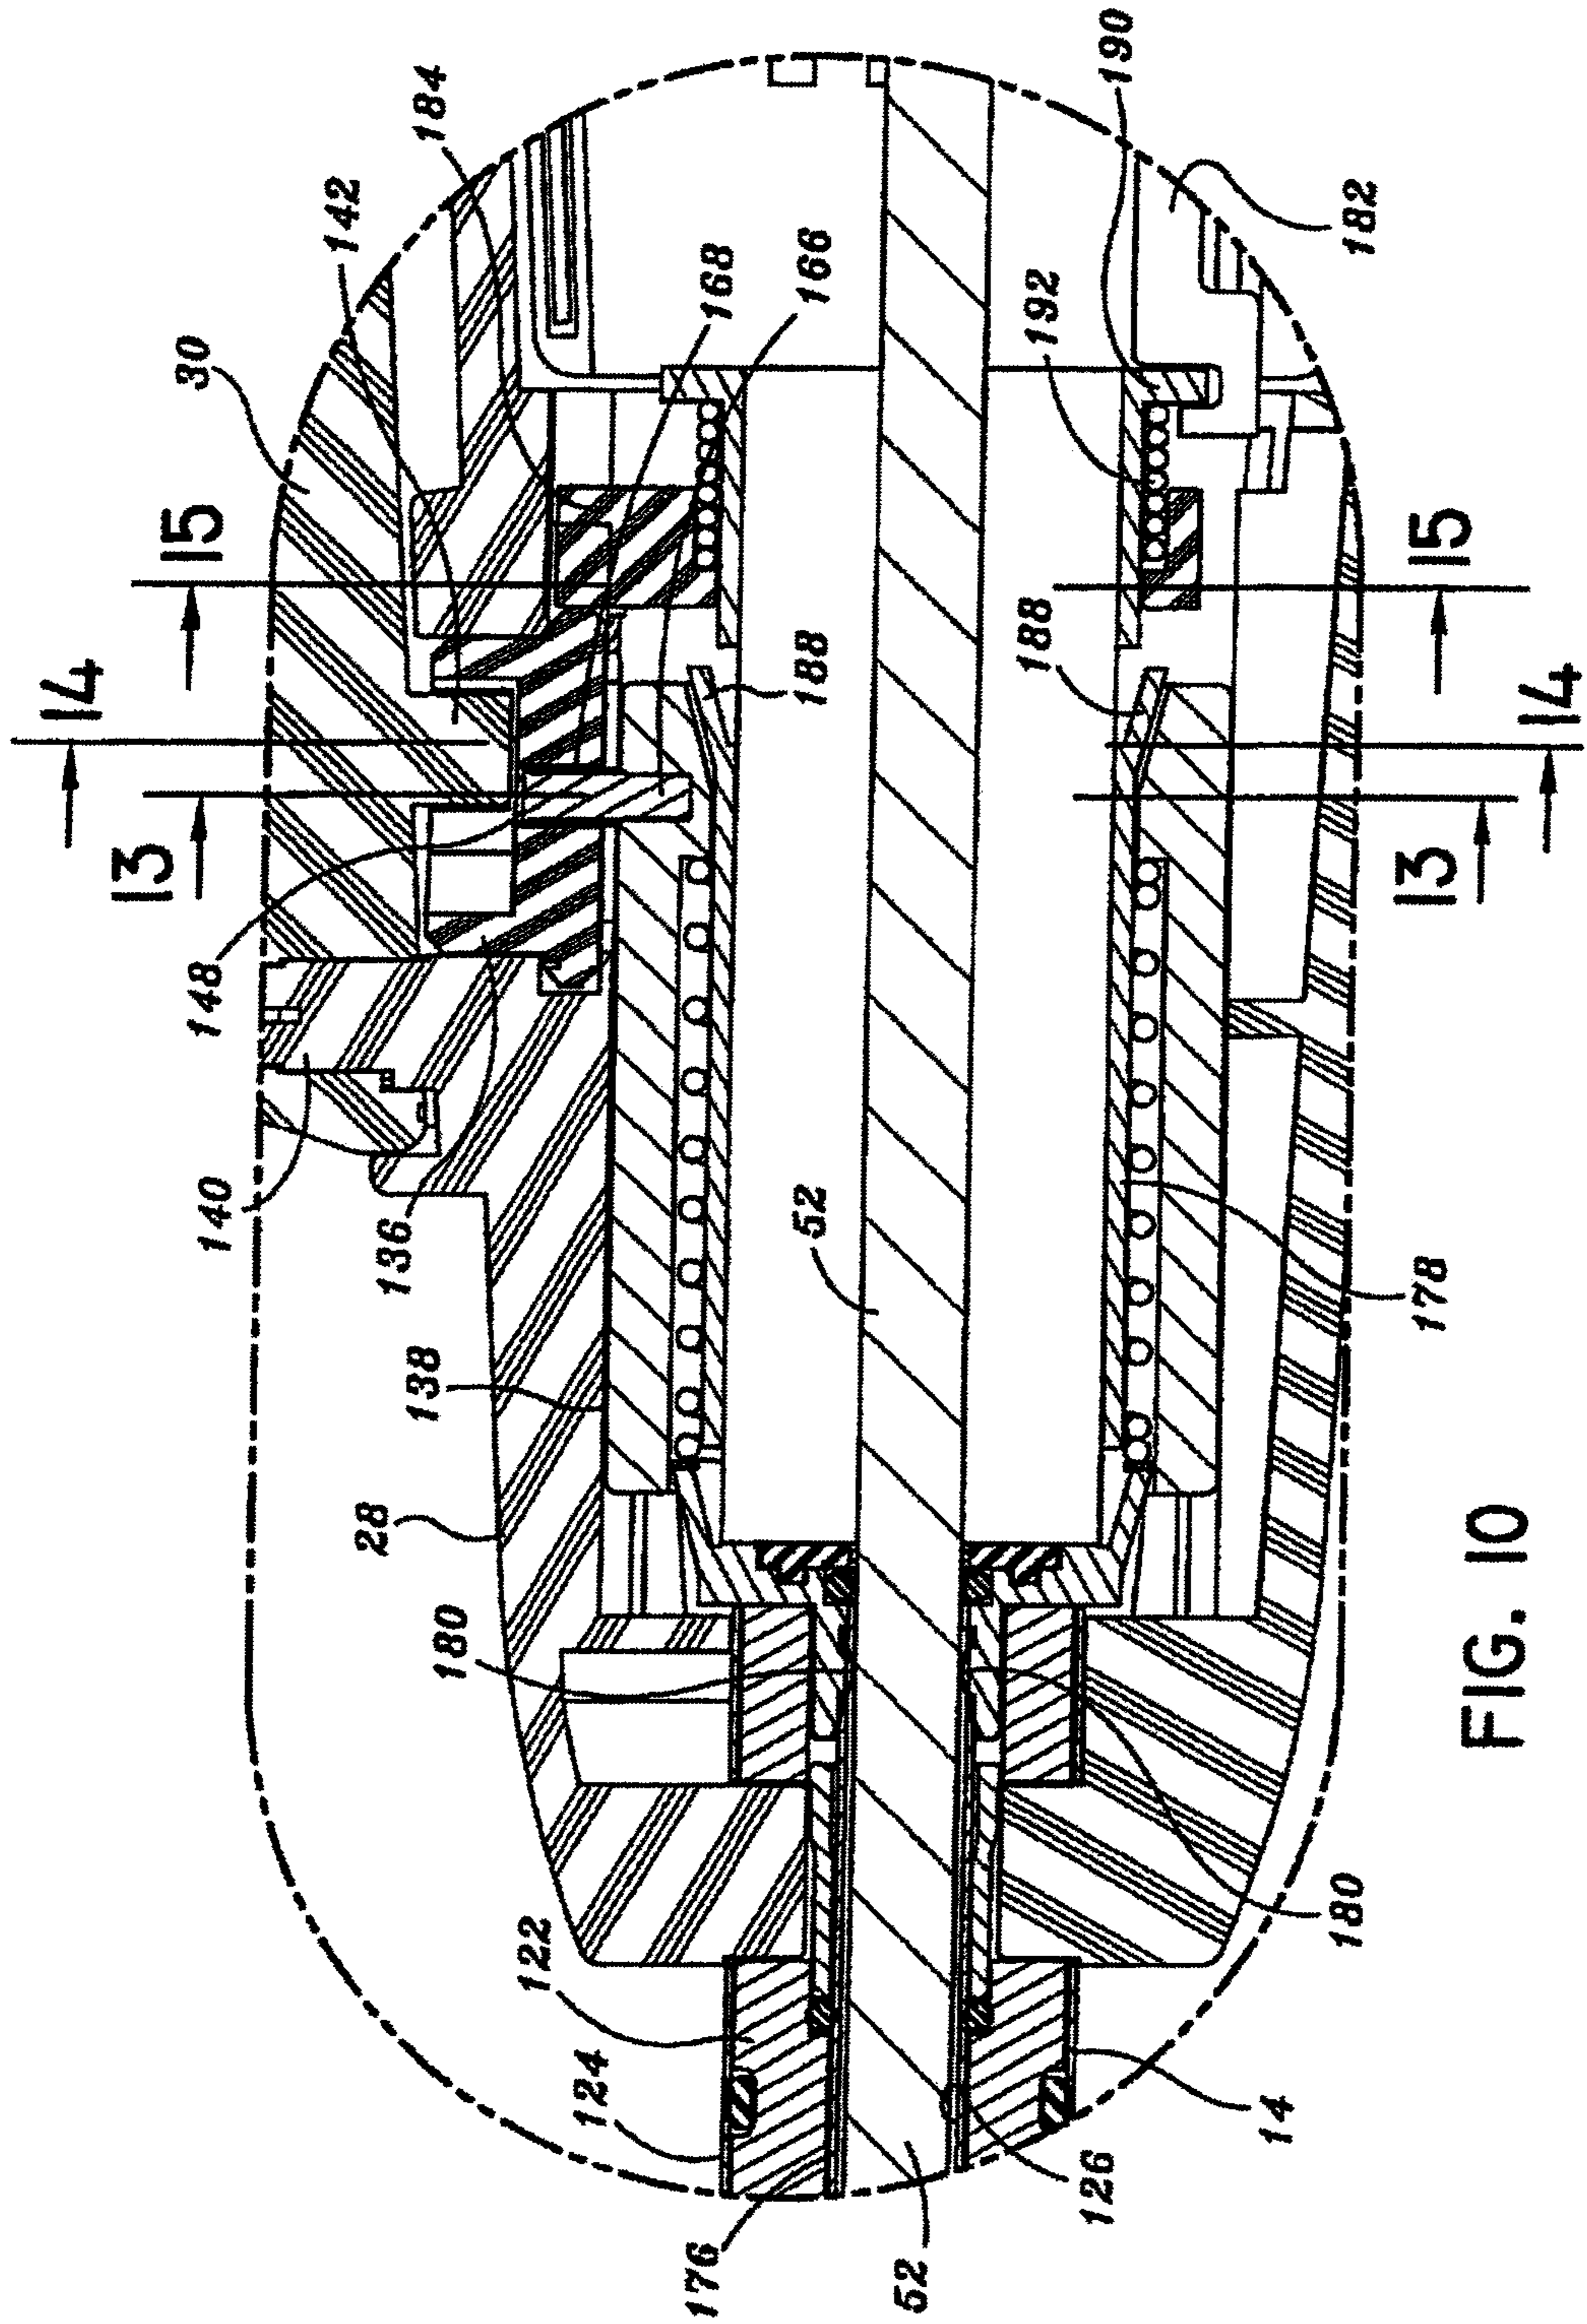


FIG. 10

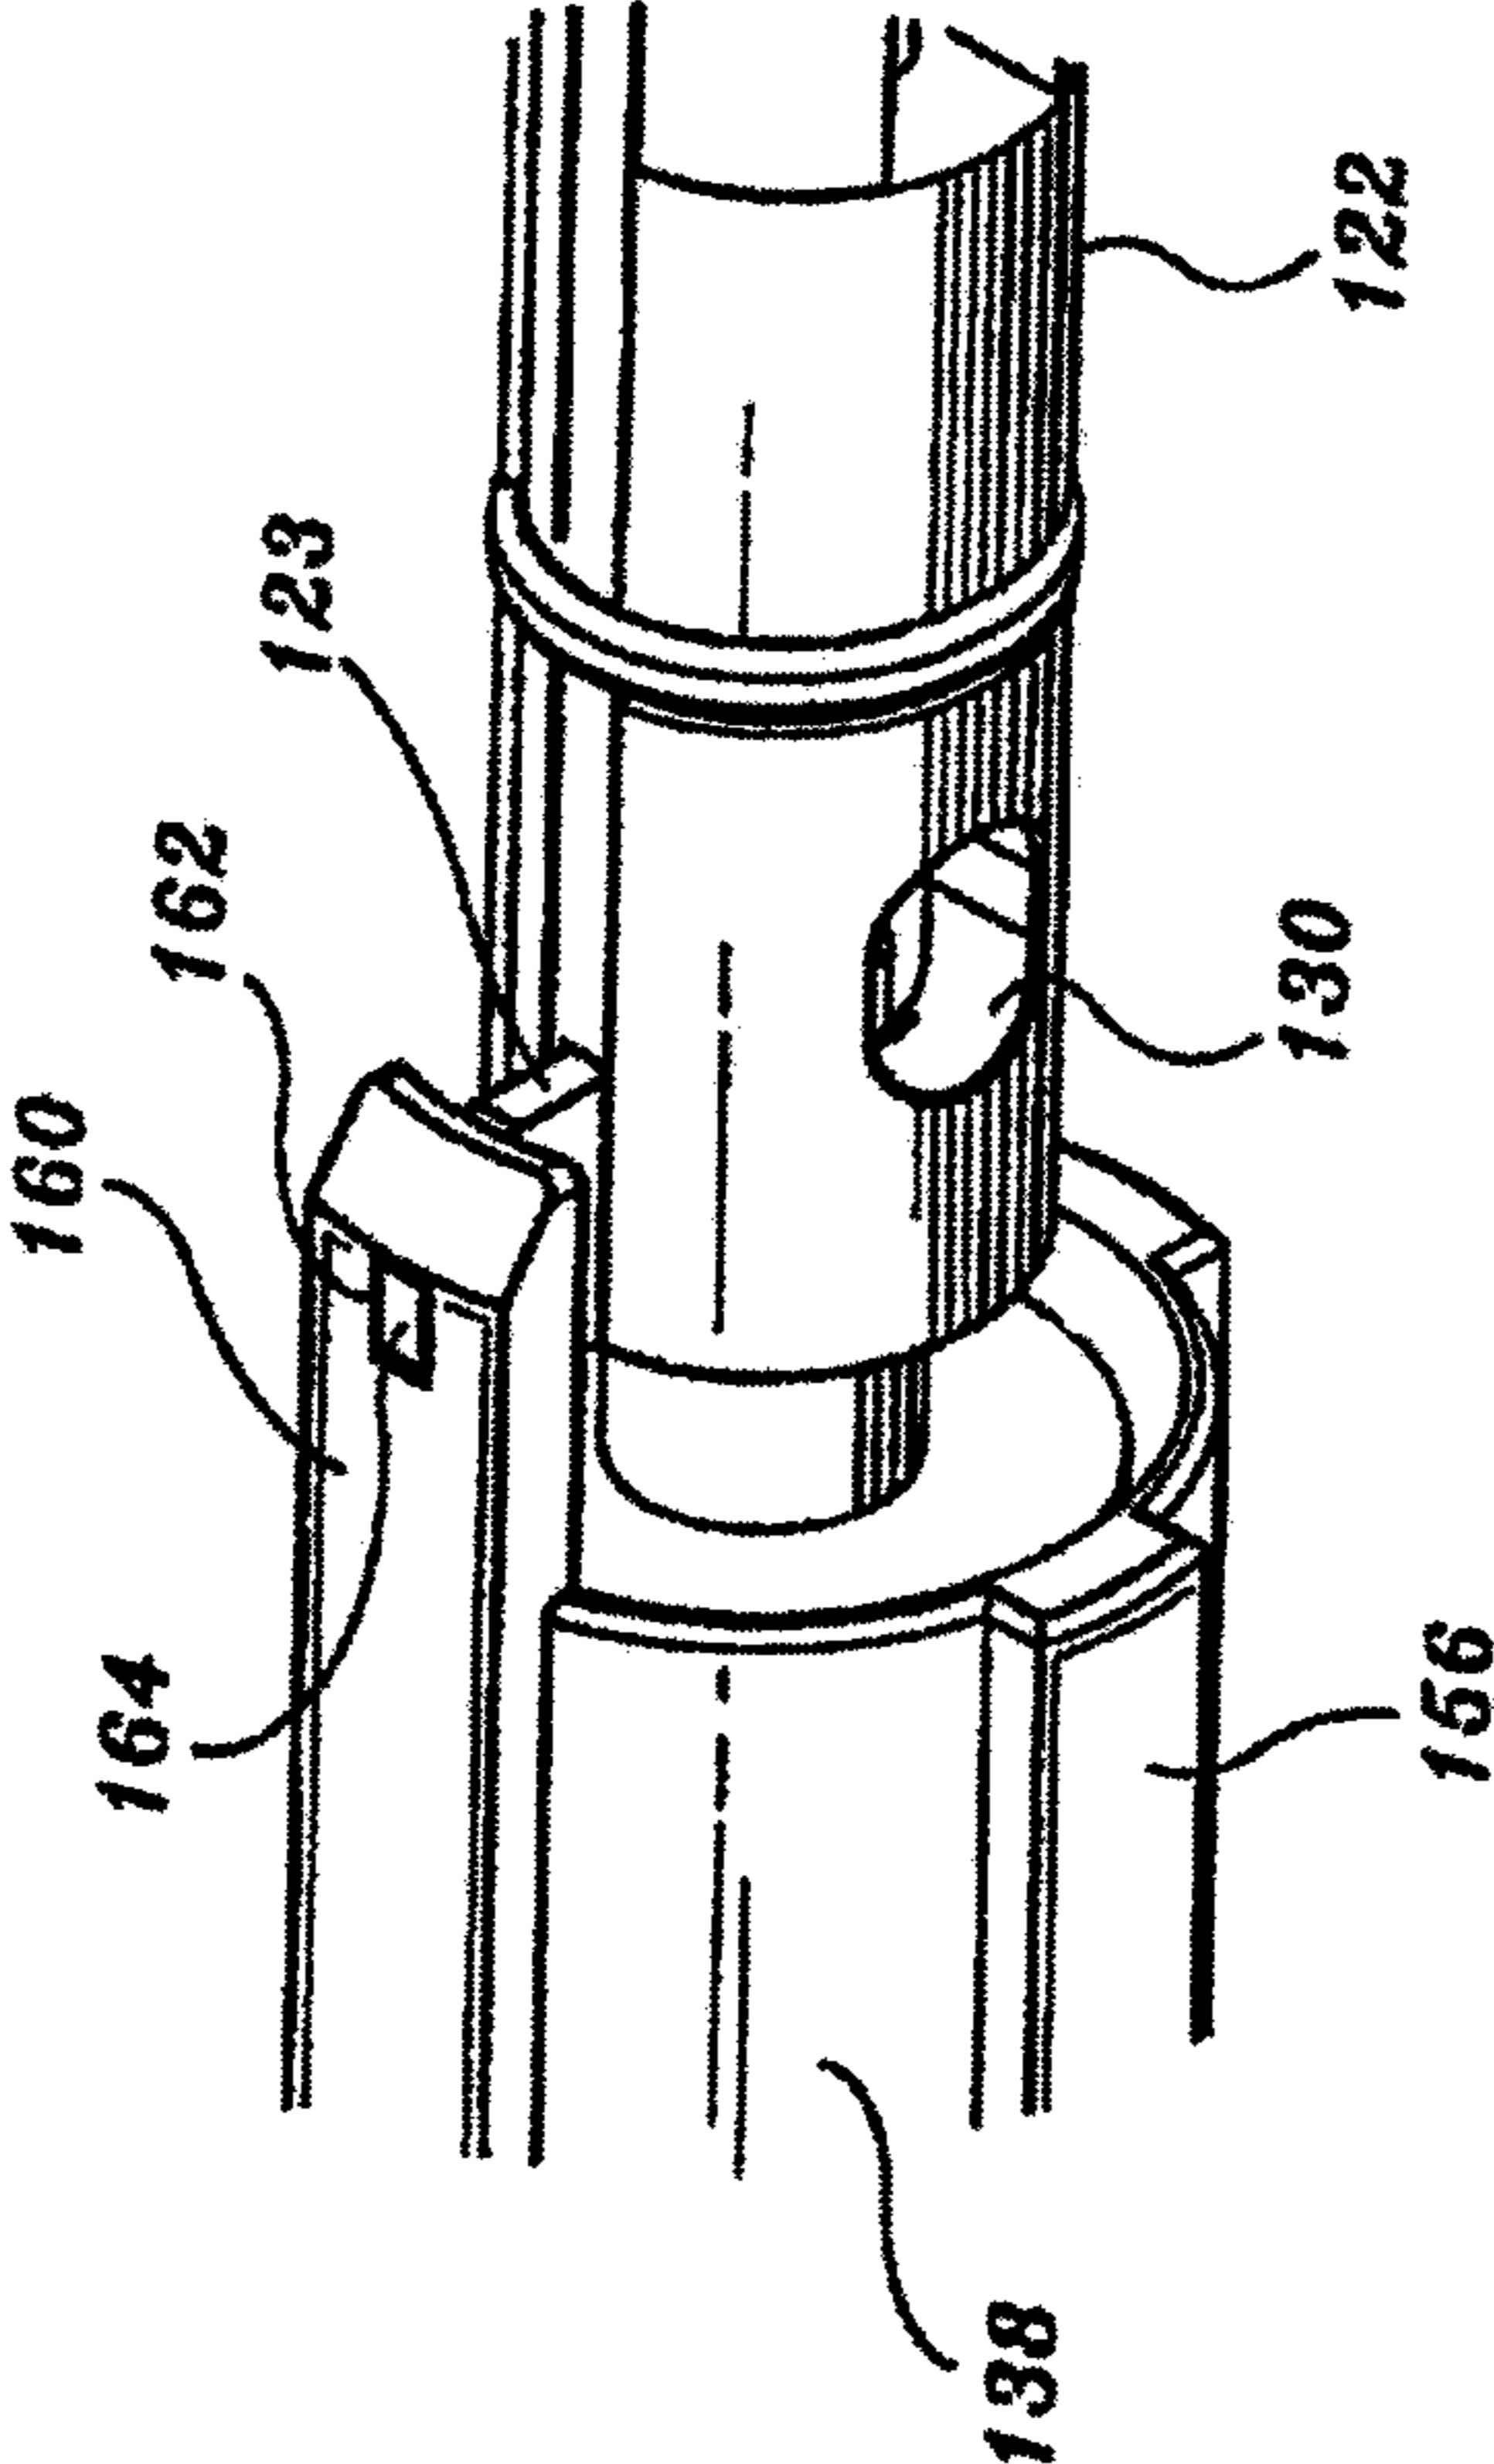


FIG. 10A



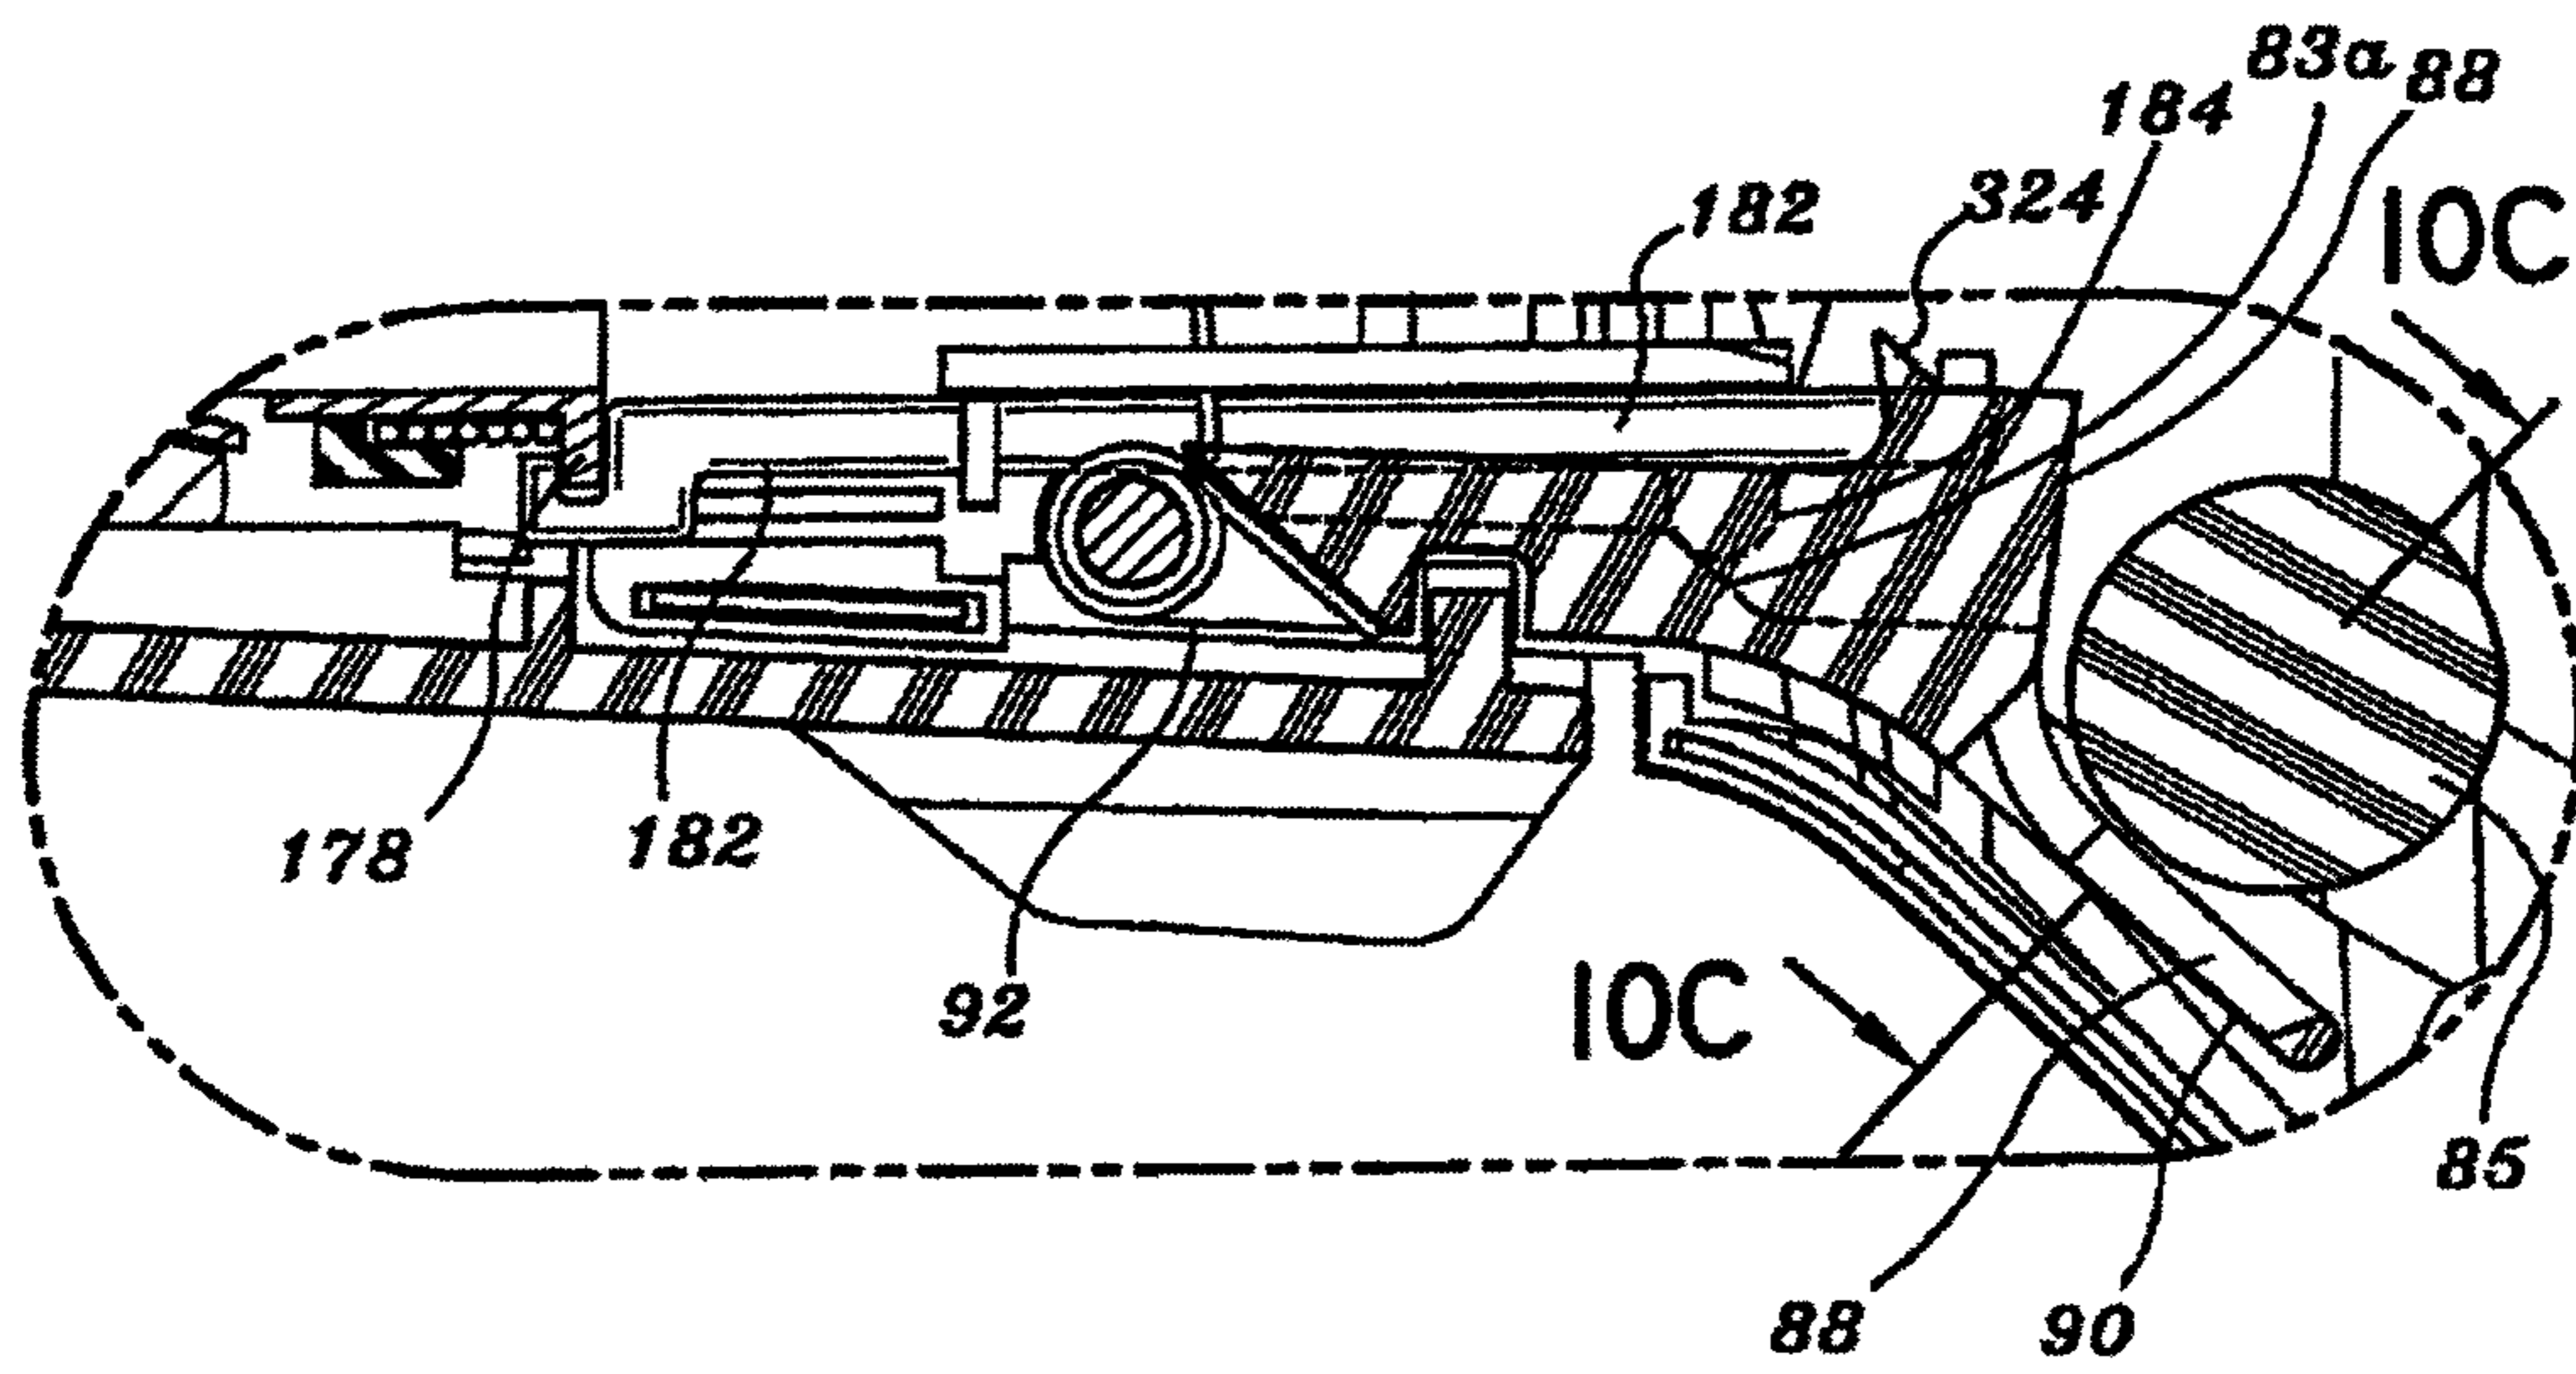


FIG. 10B

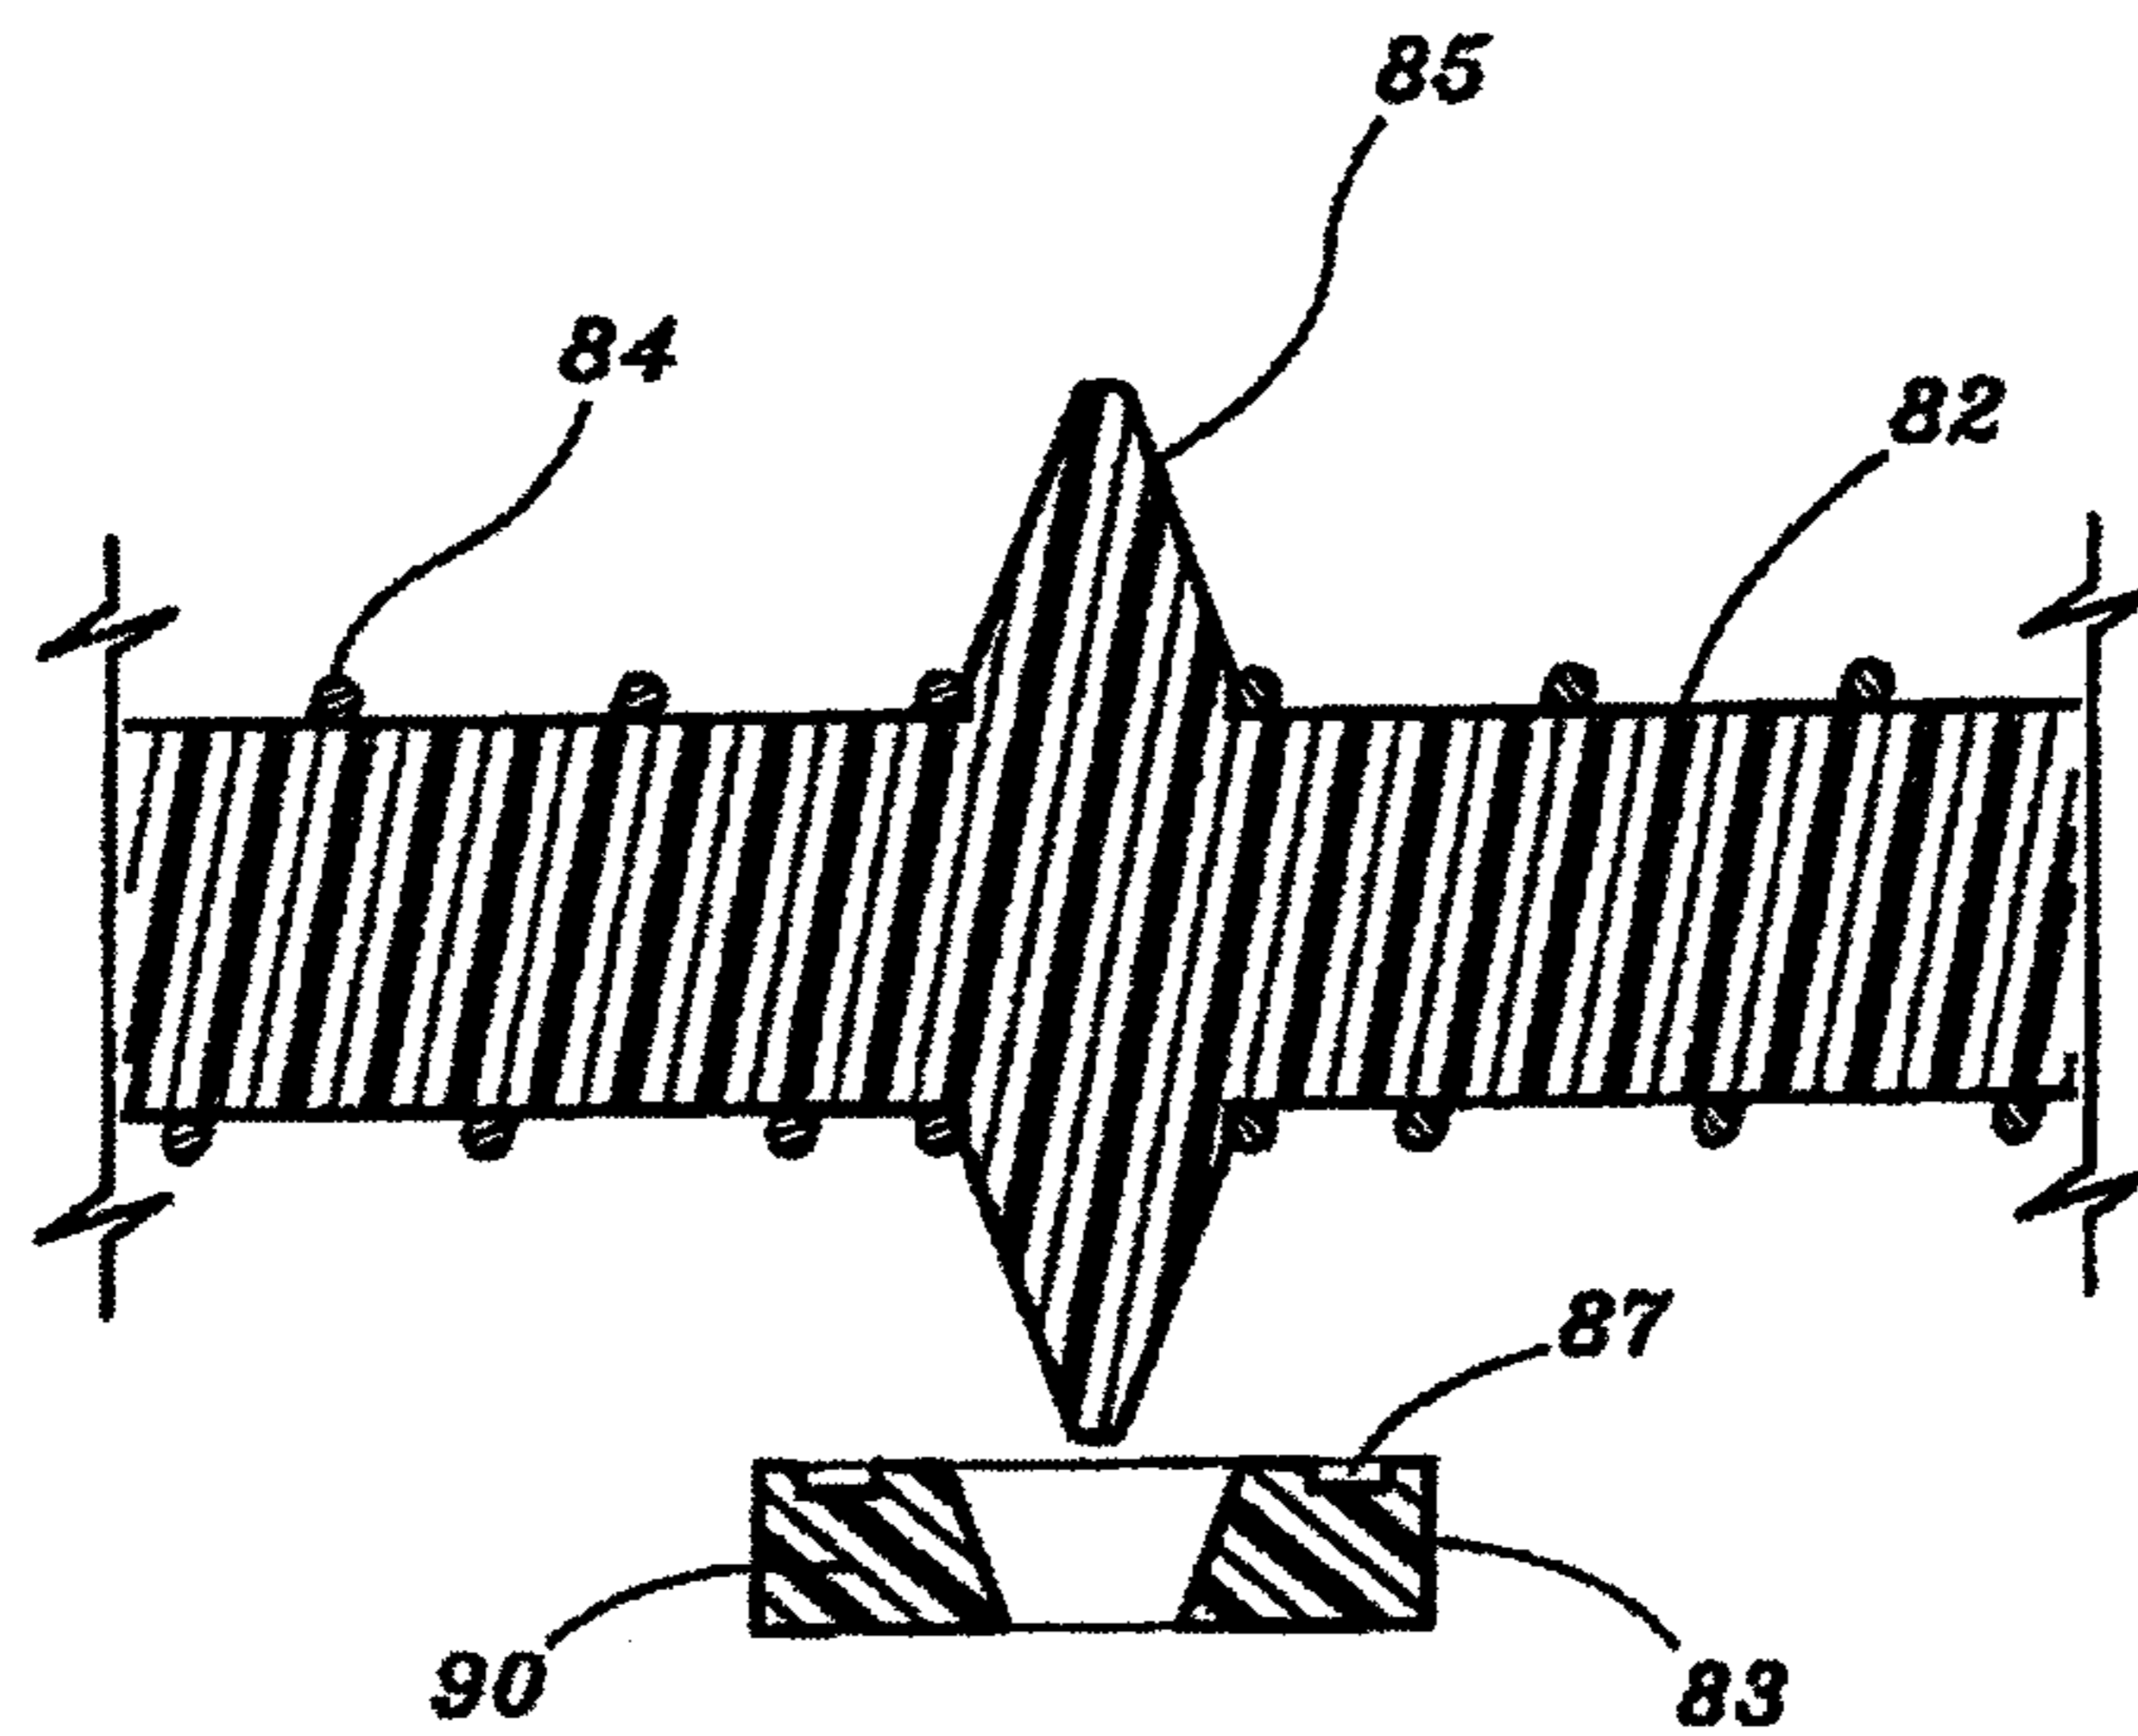


FIG. 10C

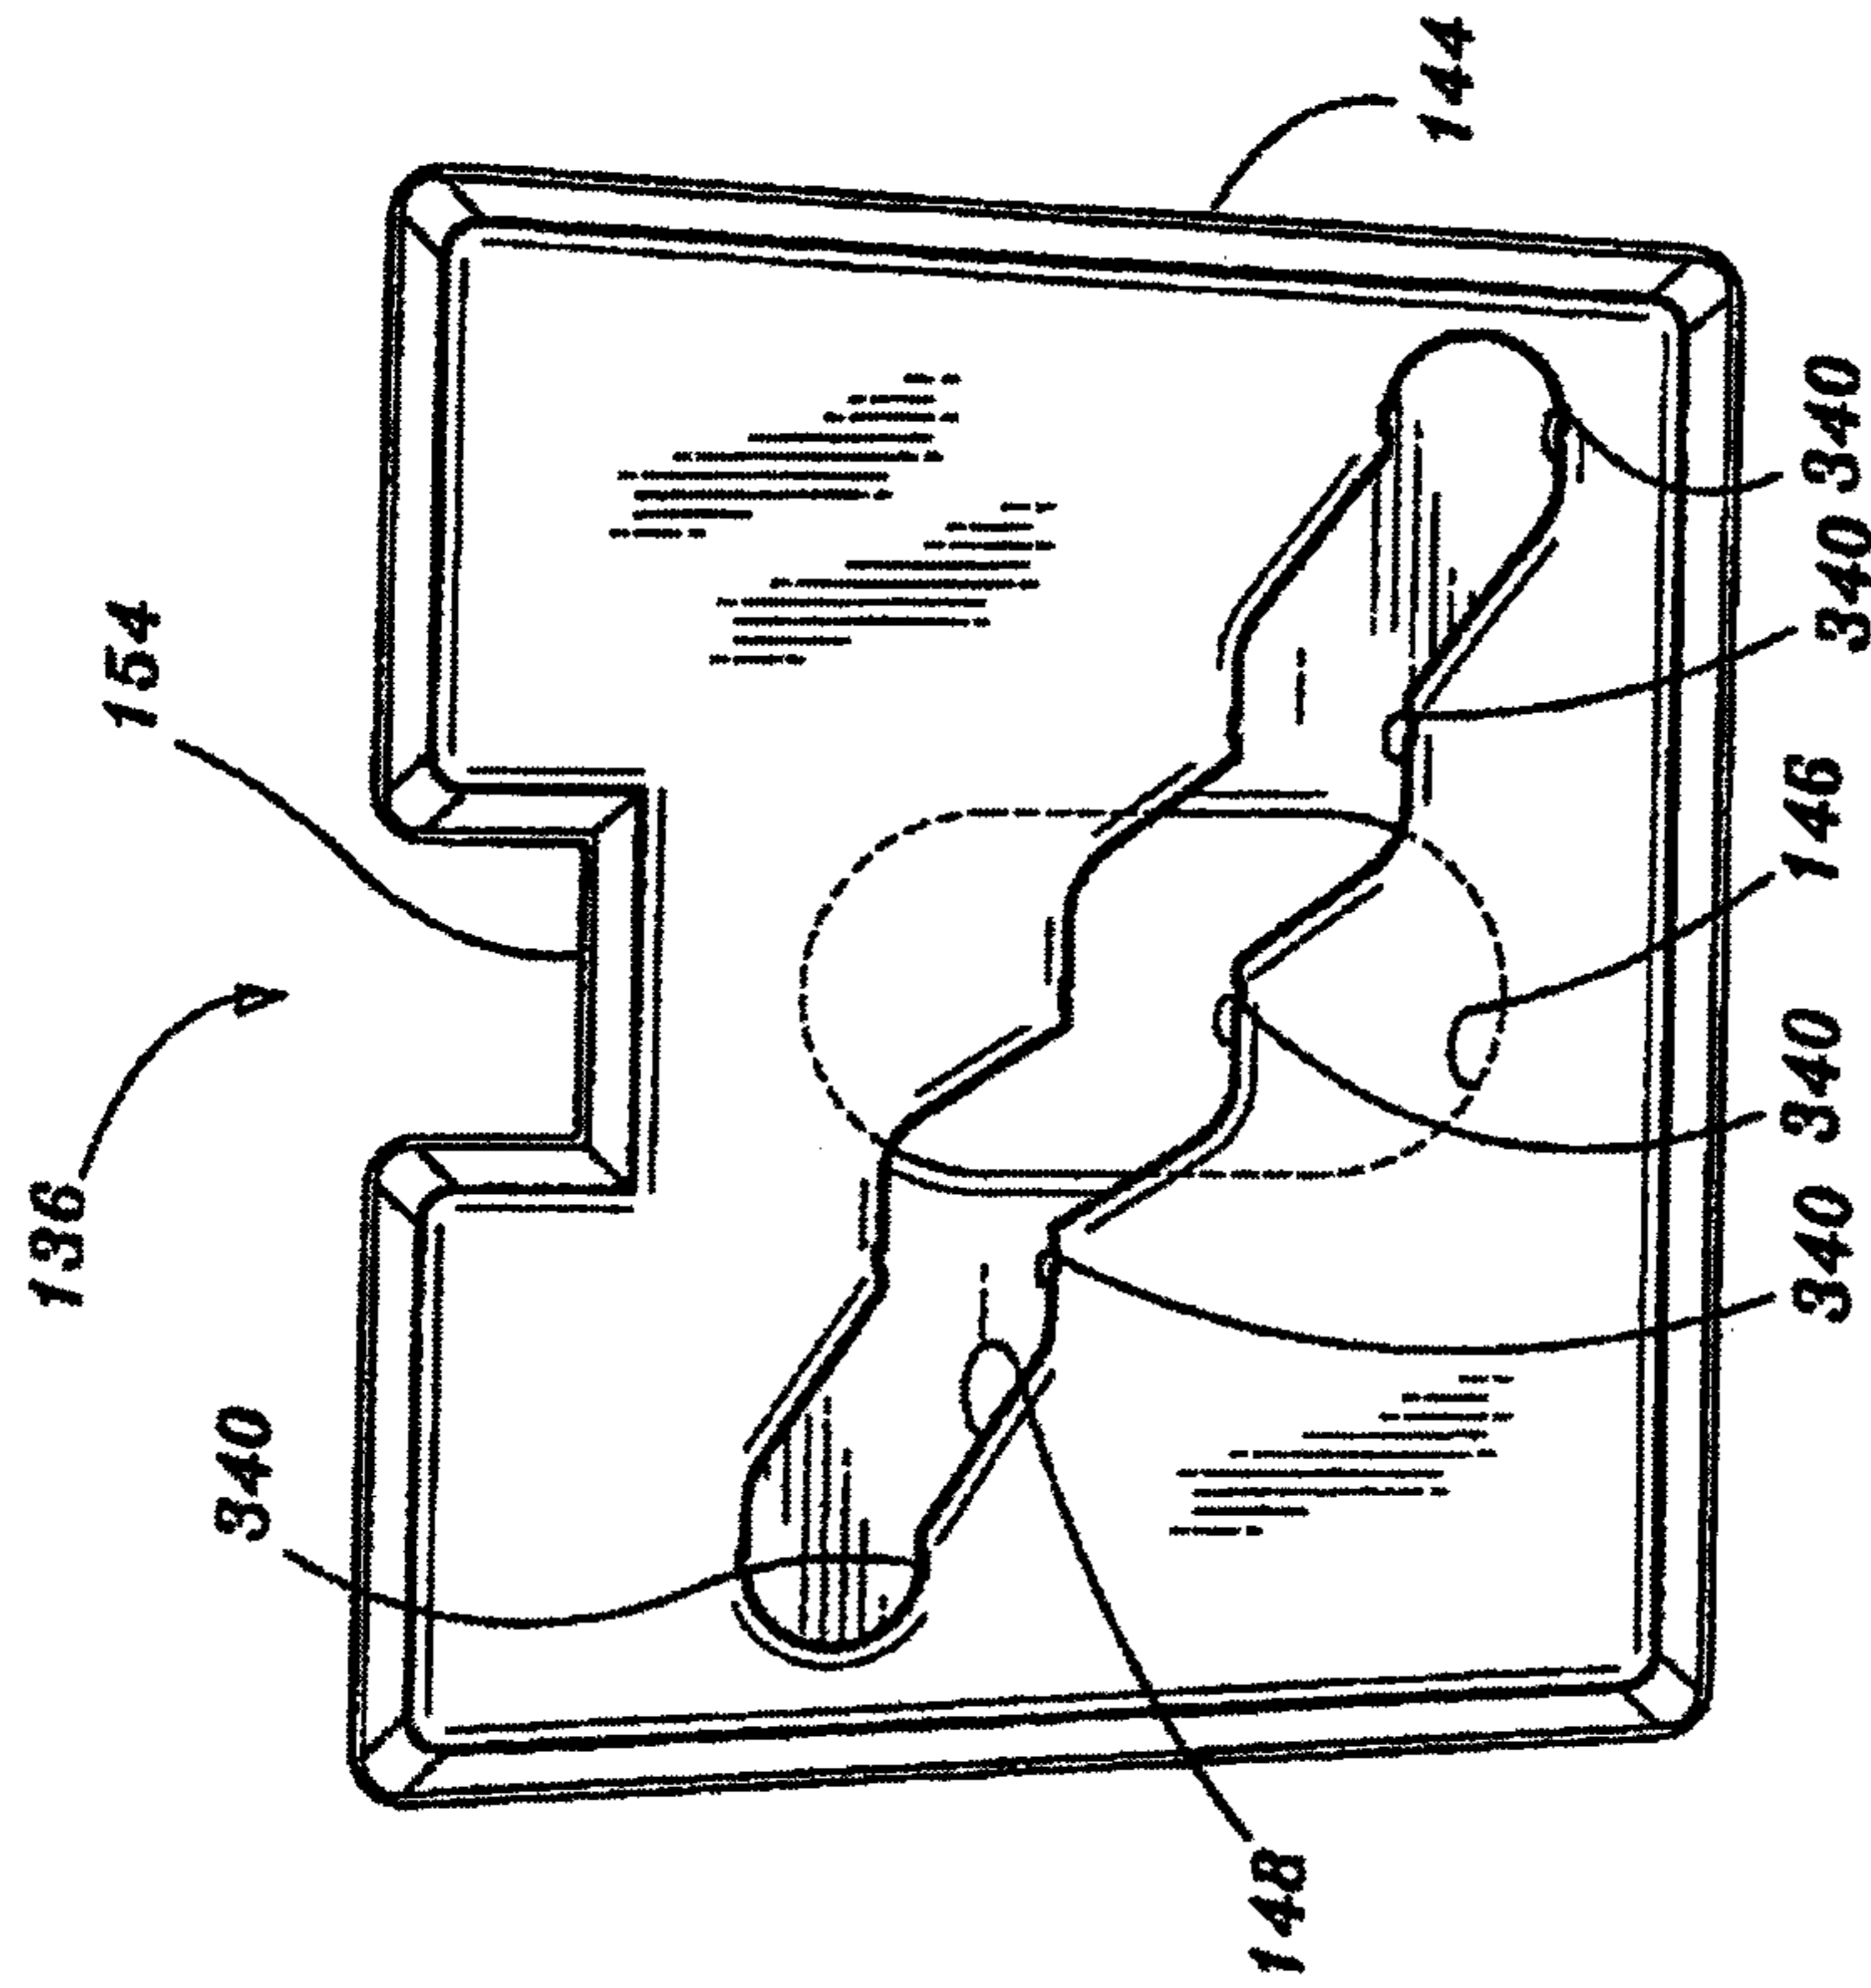


FIG. 12

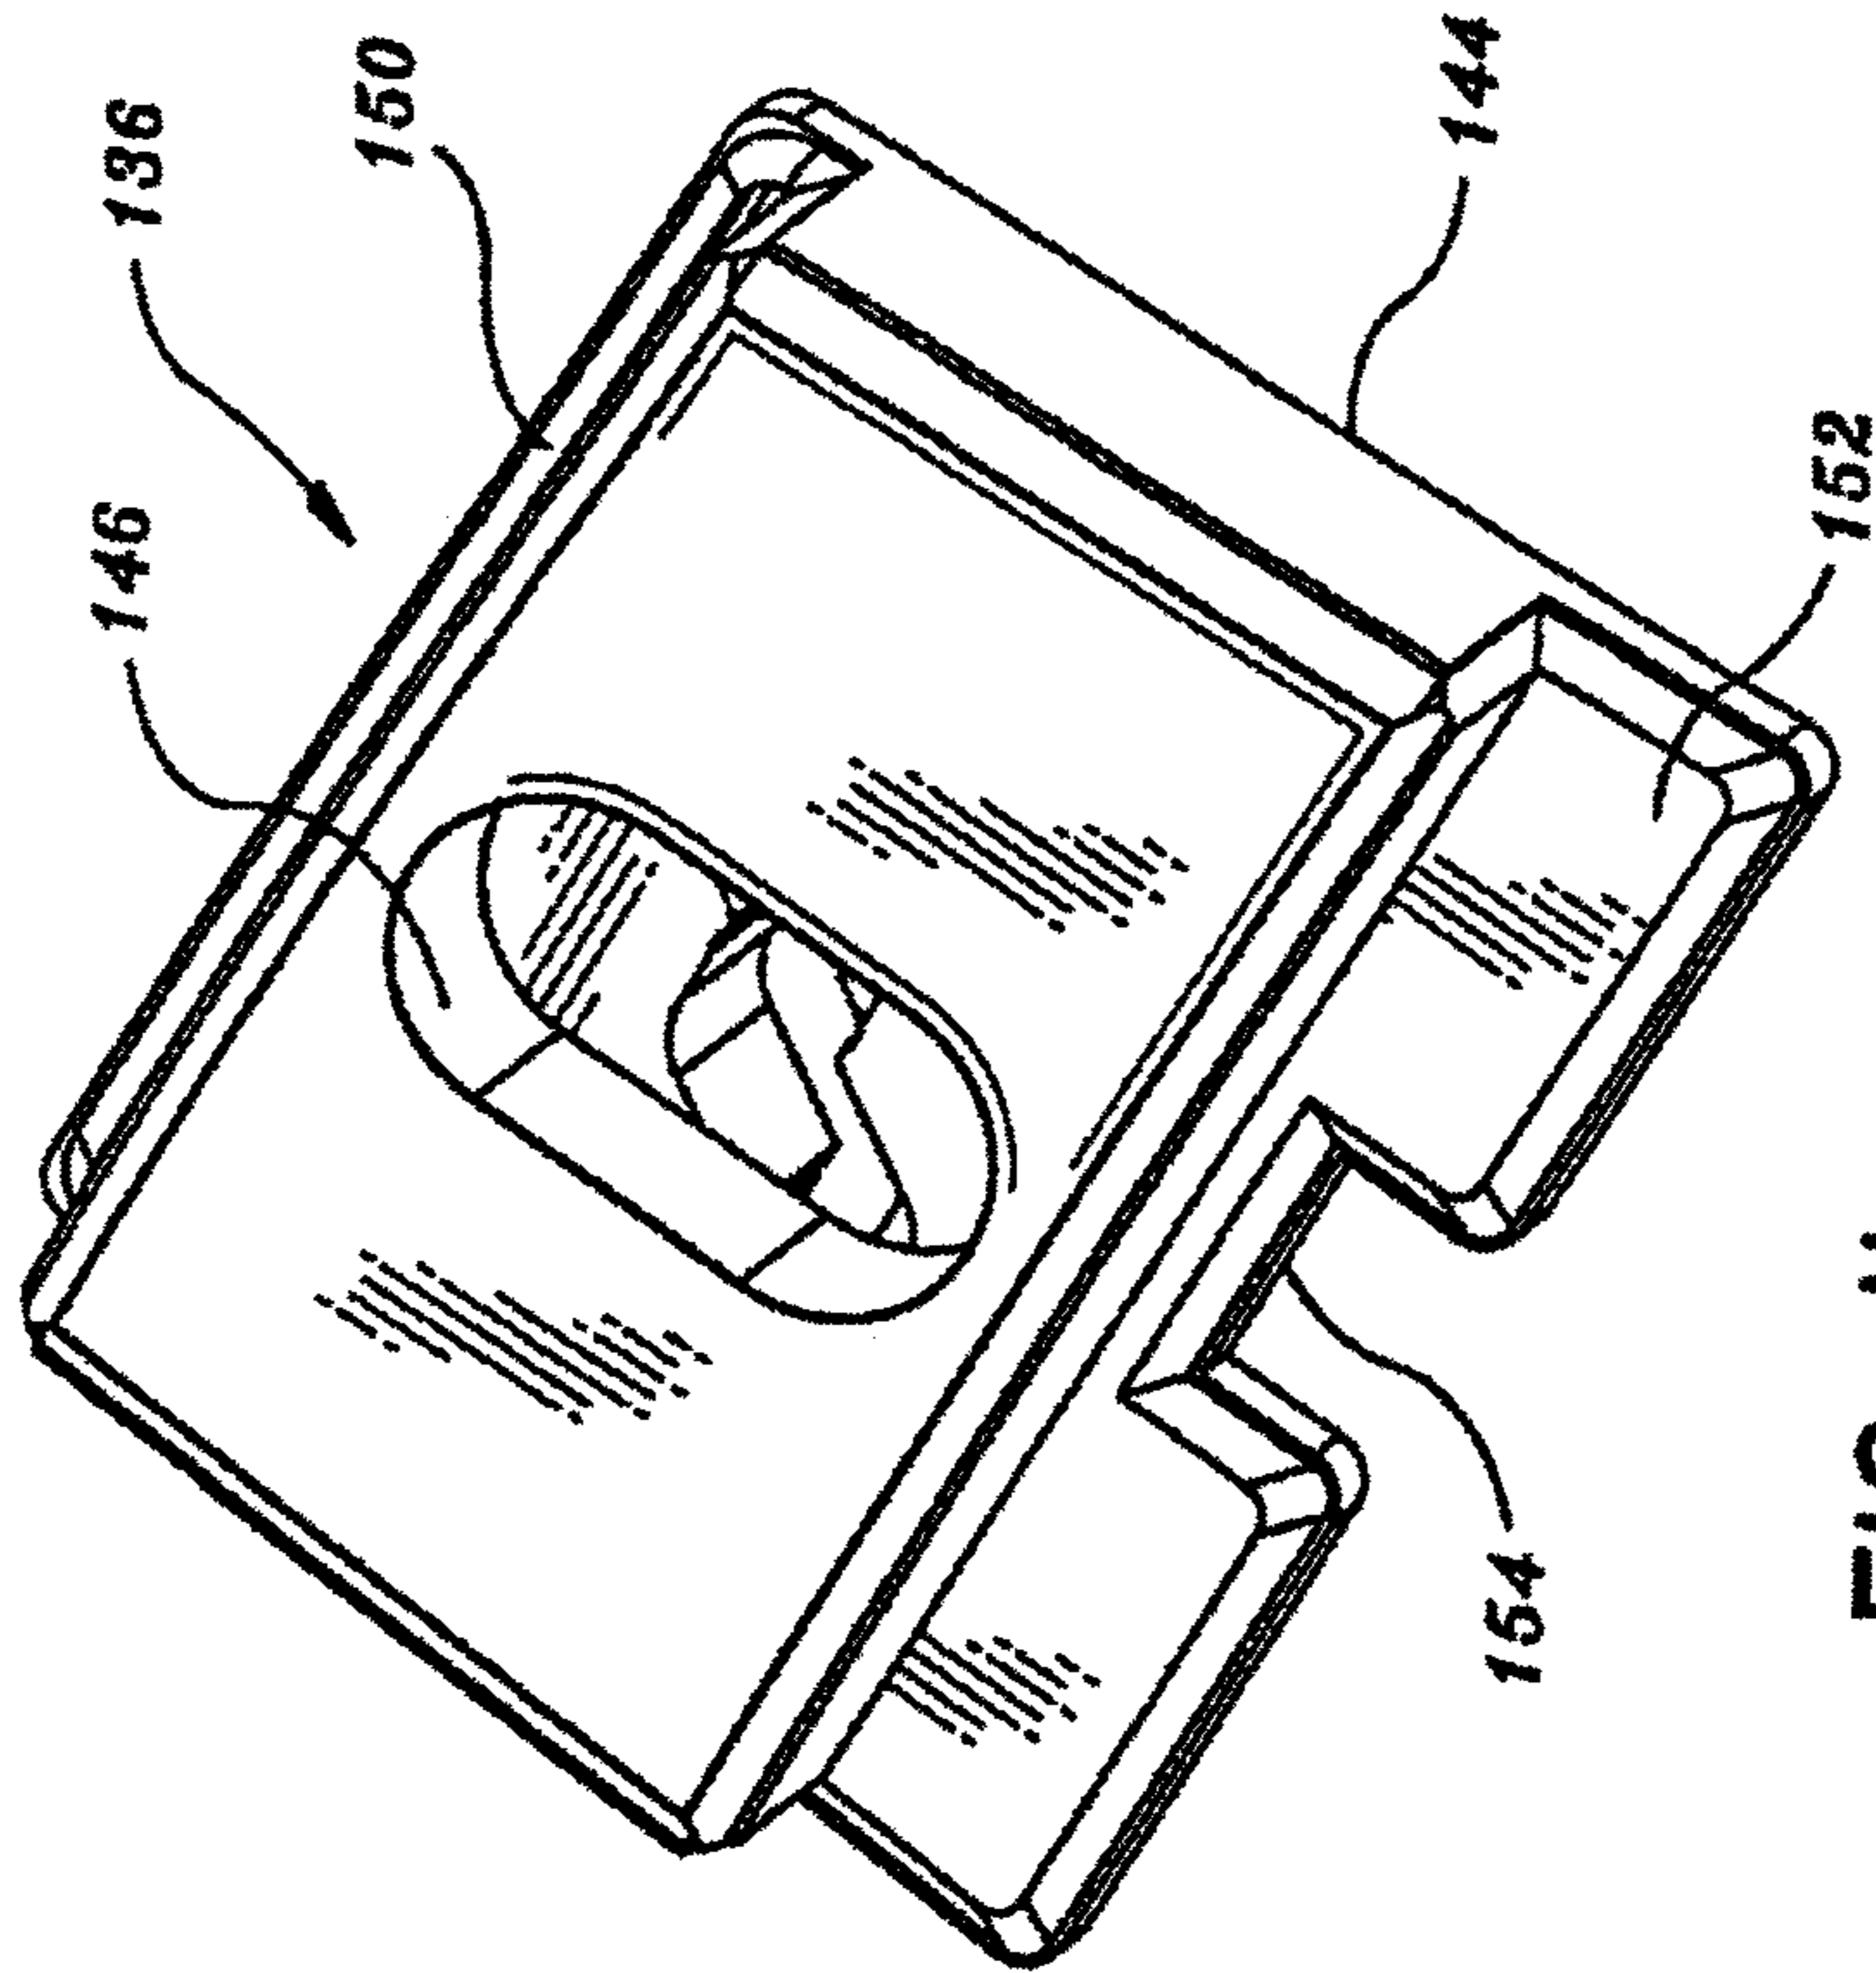


FIG. 11

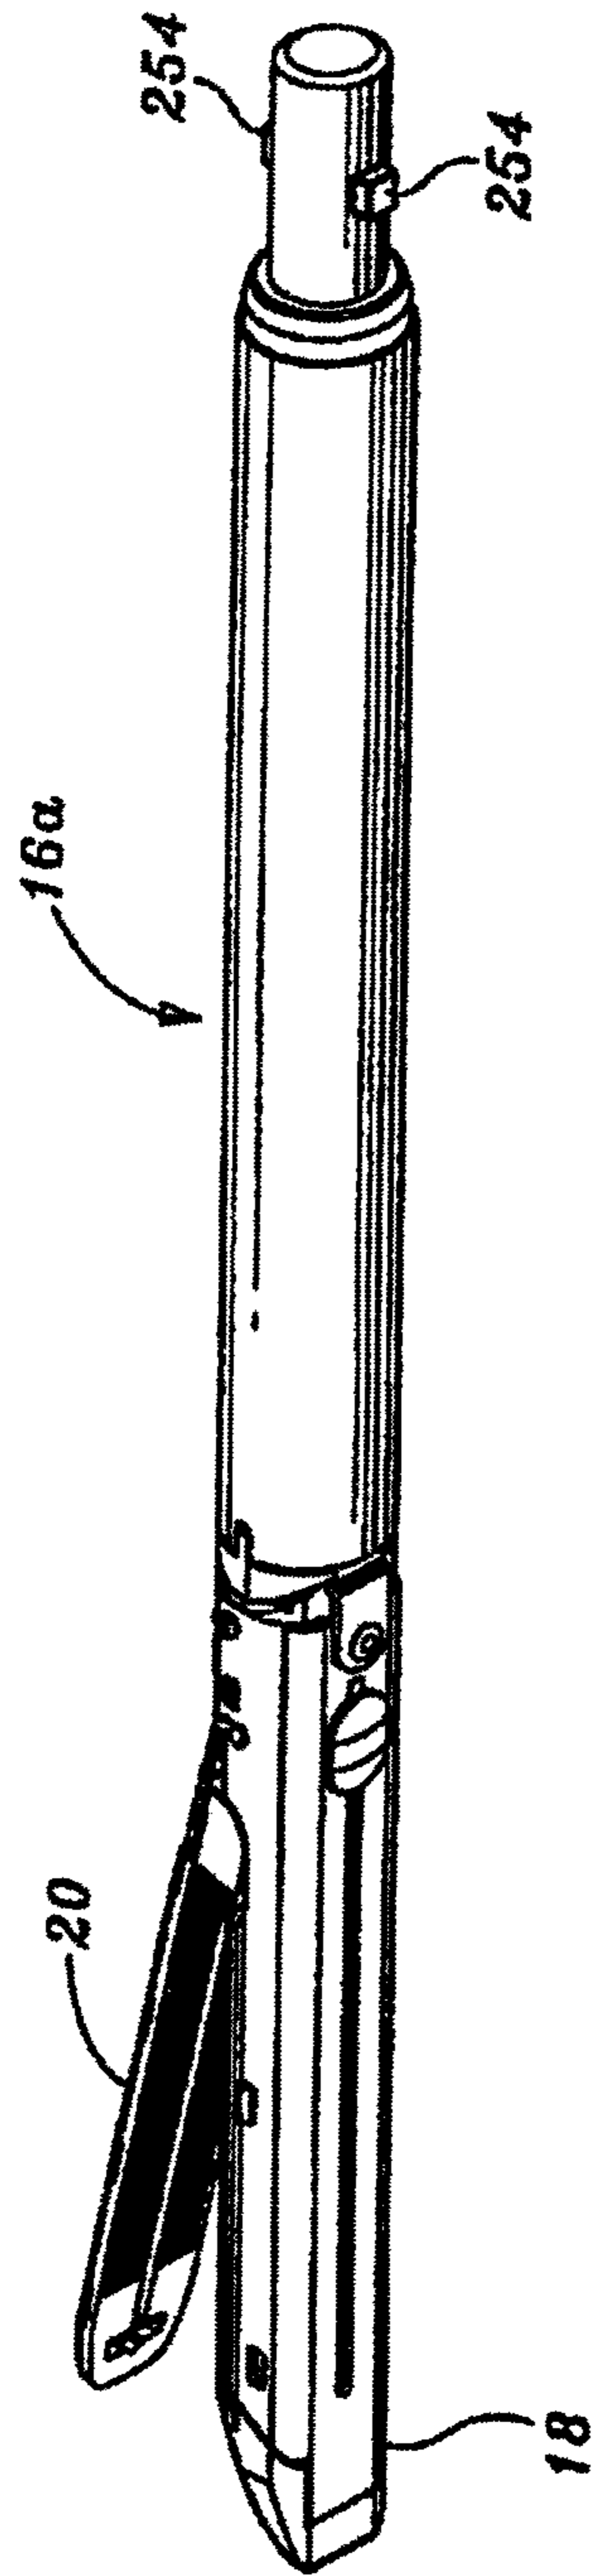


FIG. 12A

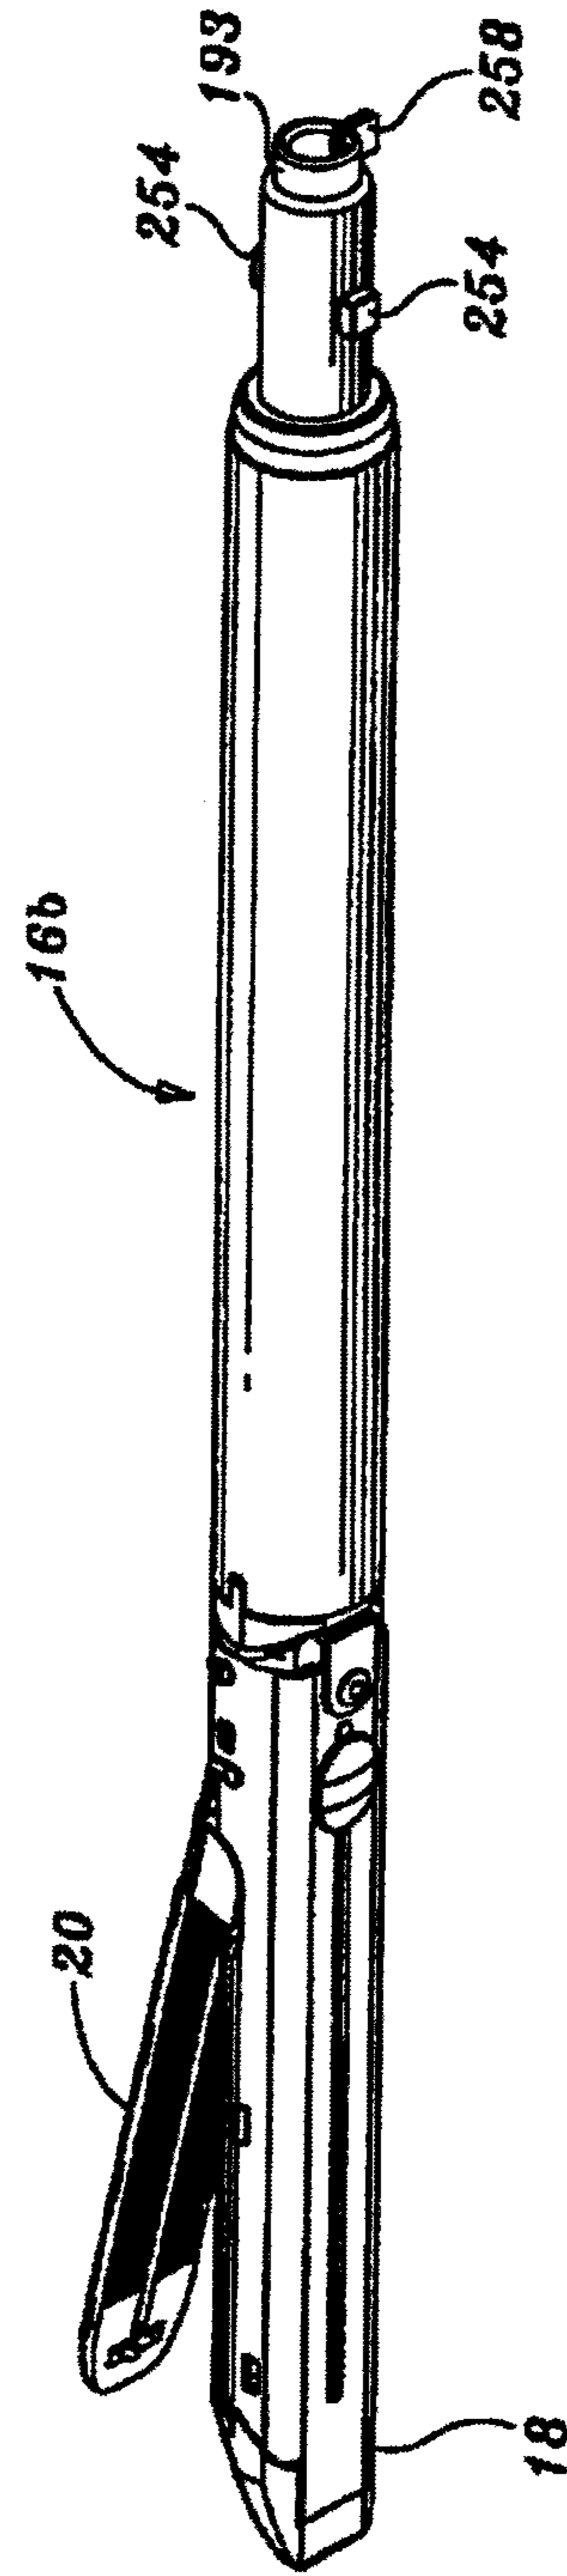


FIG. 12B

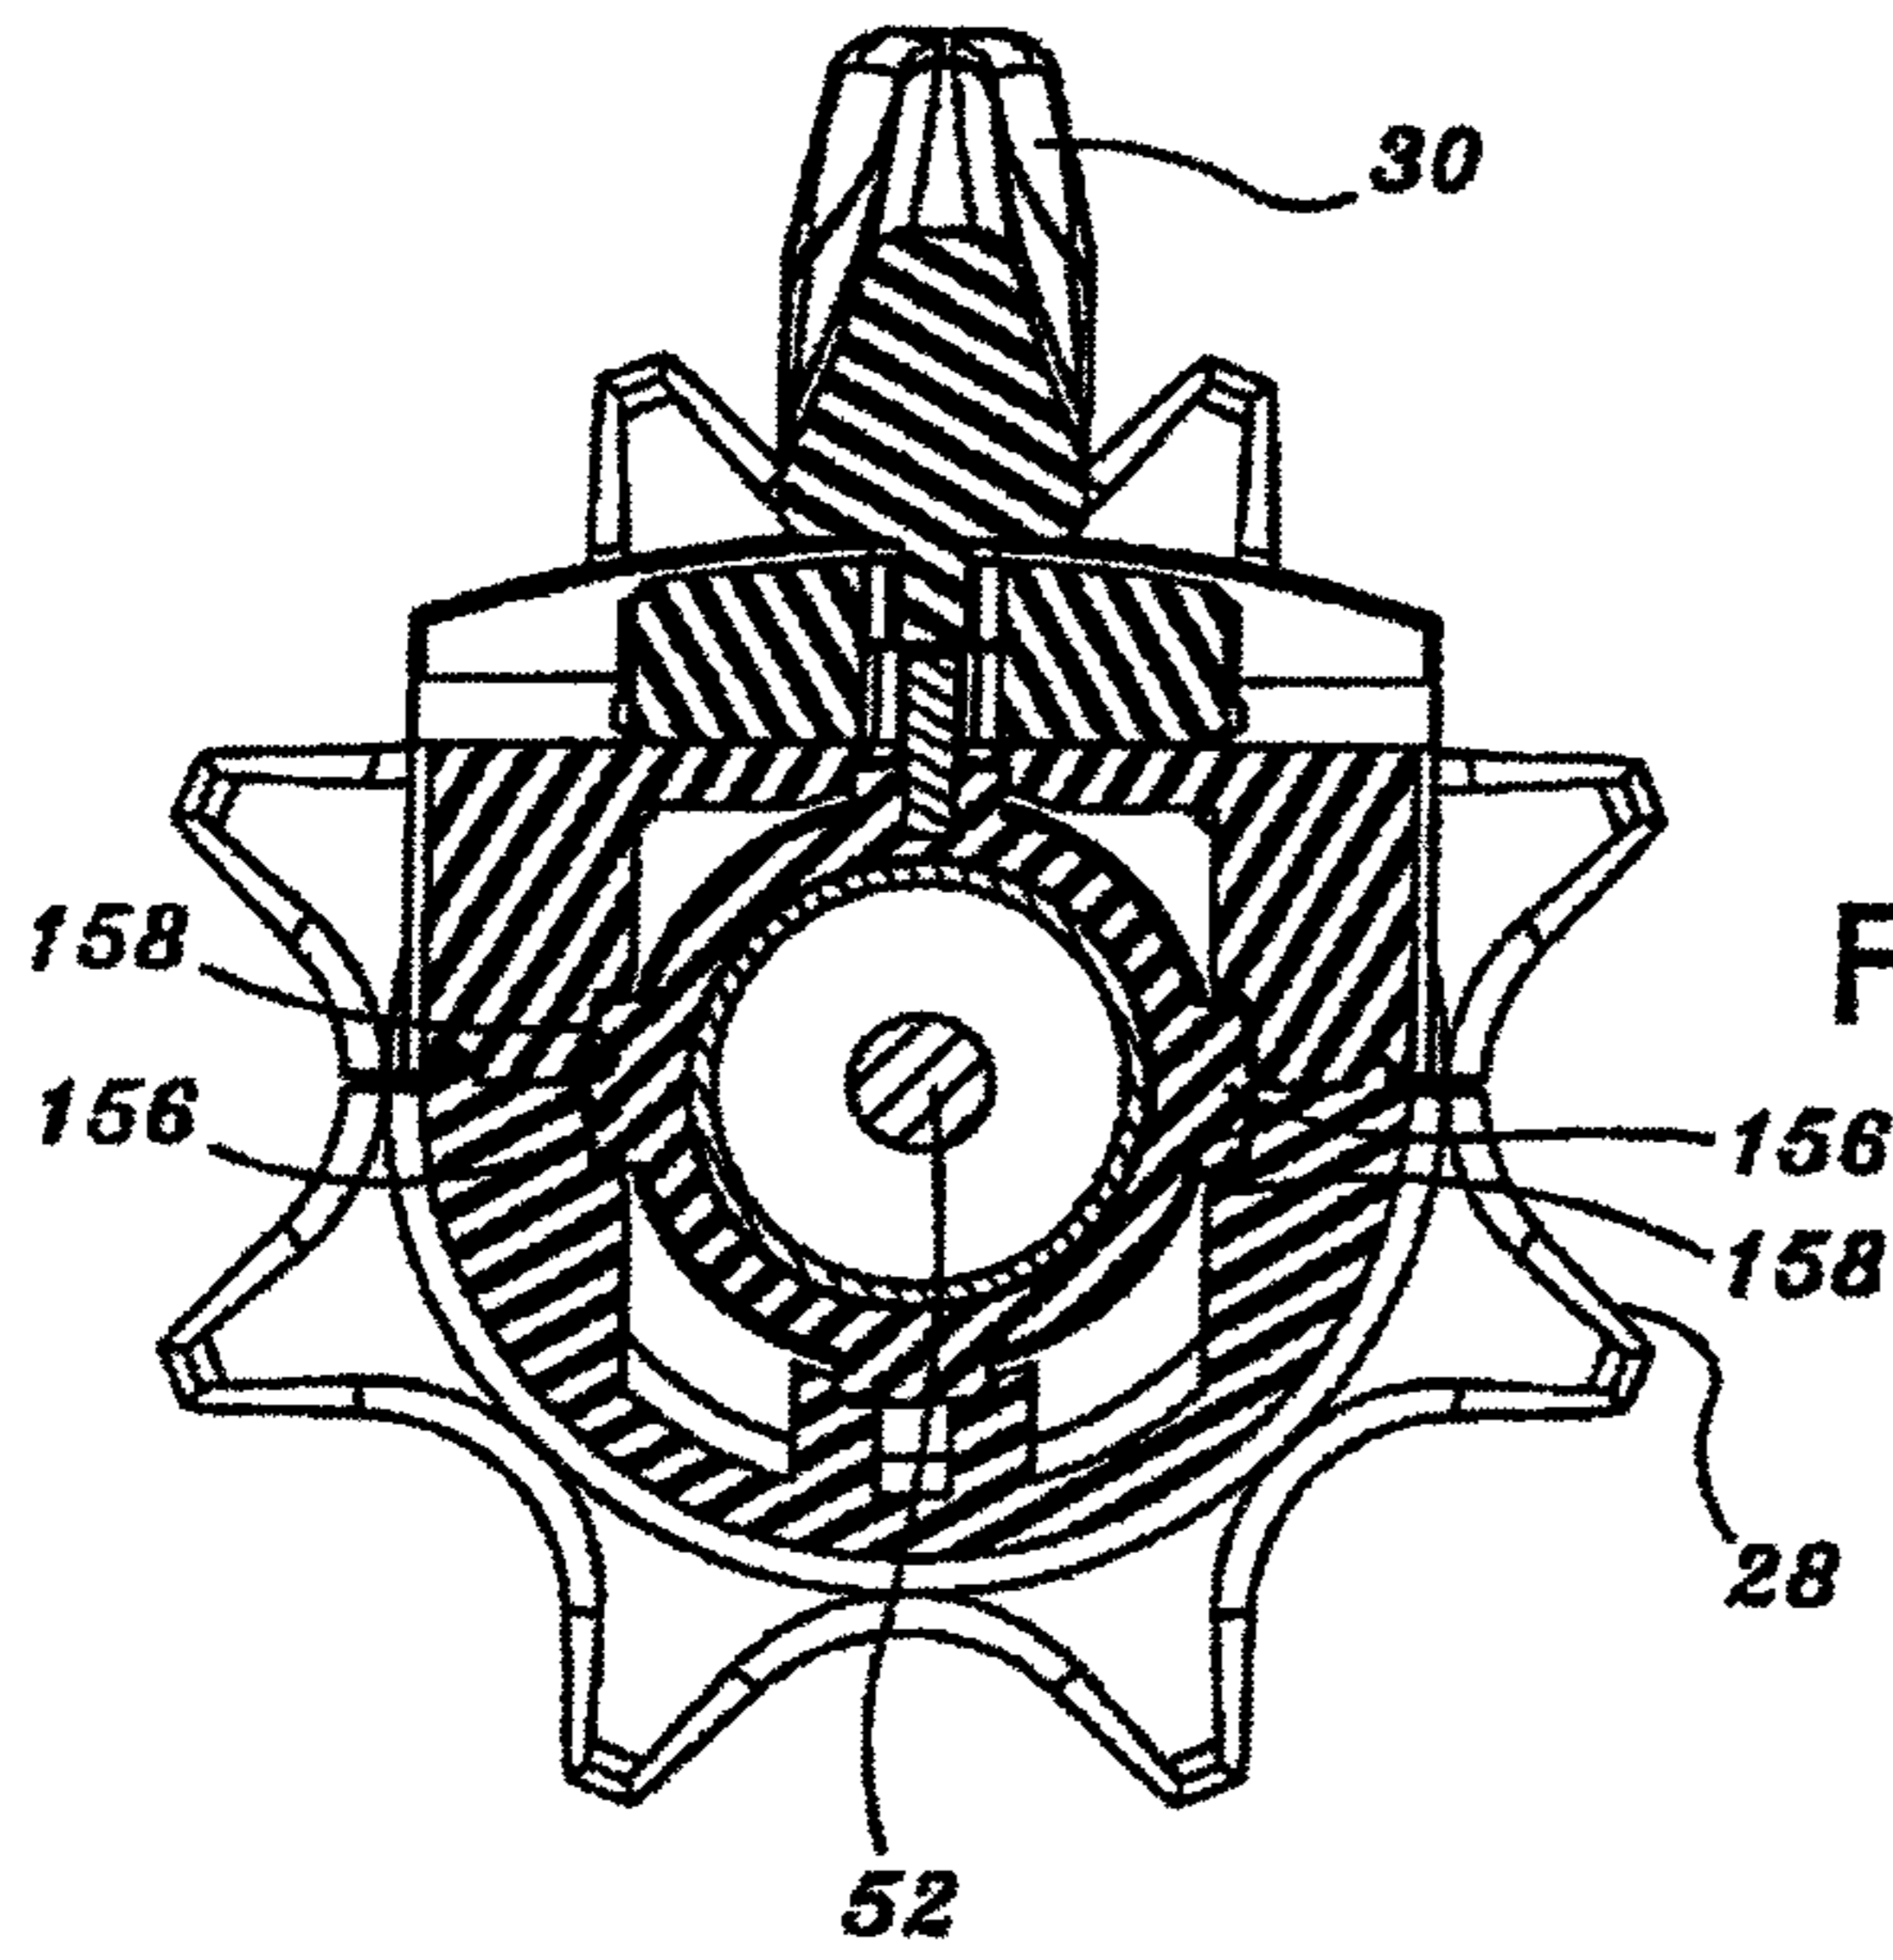


FIG. 13

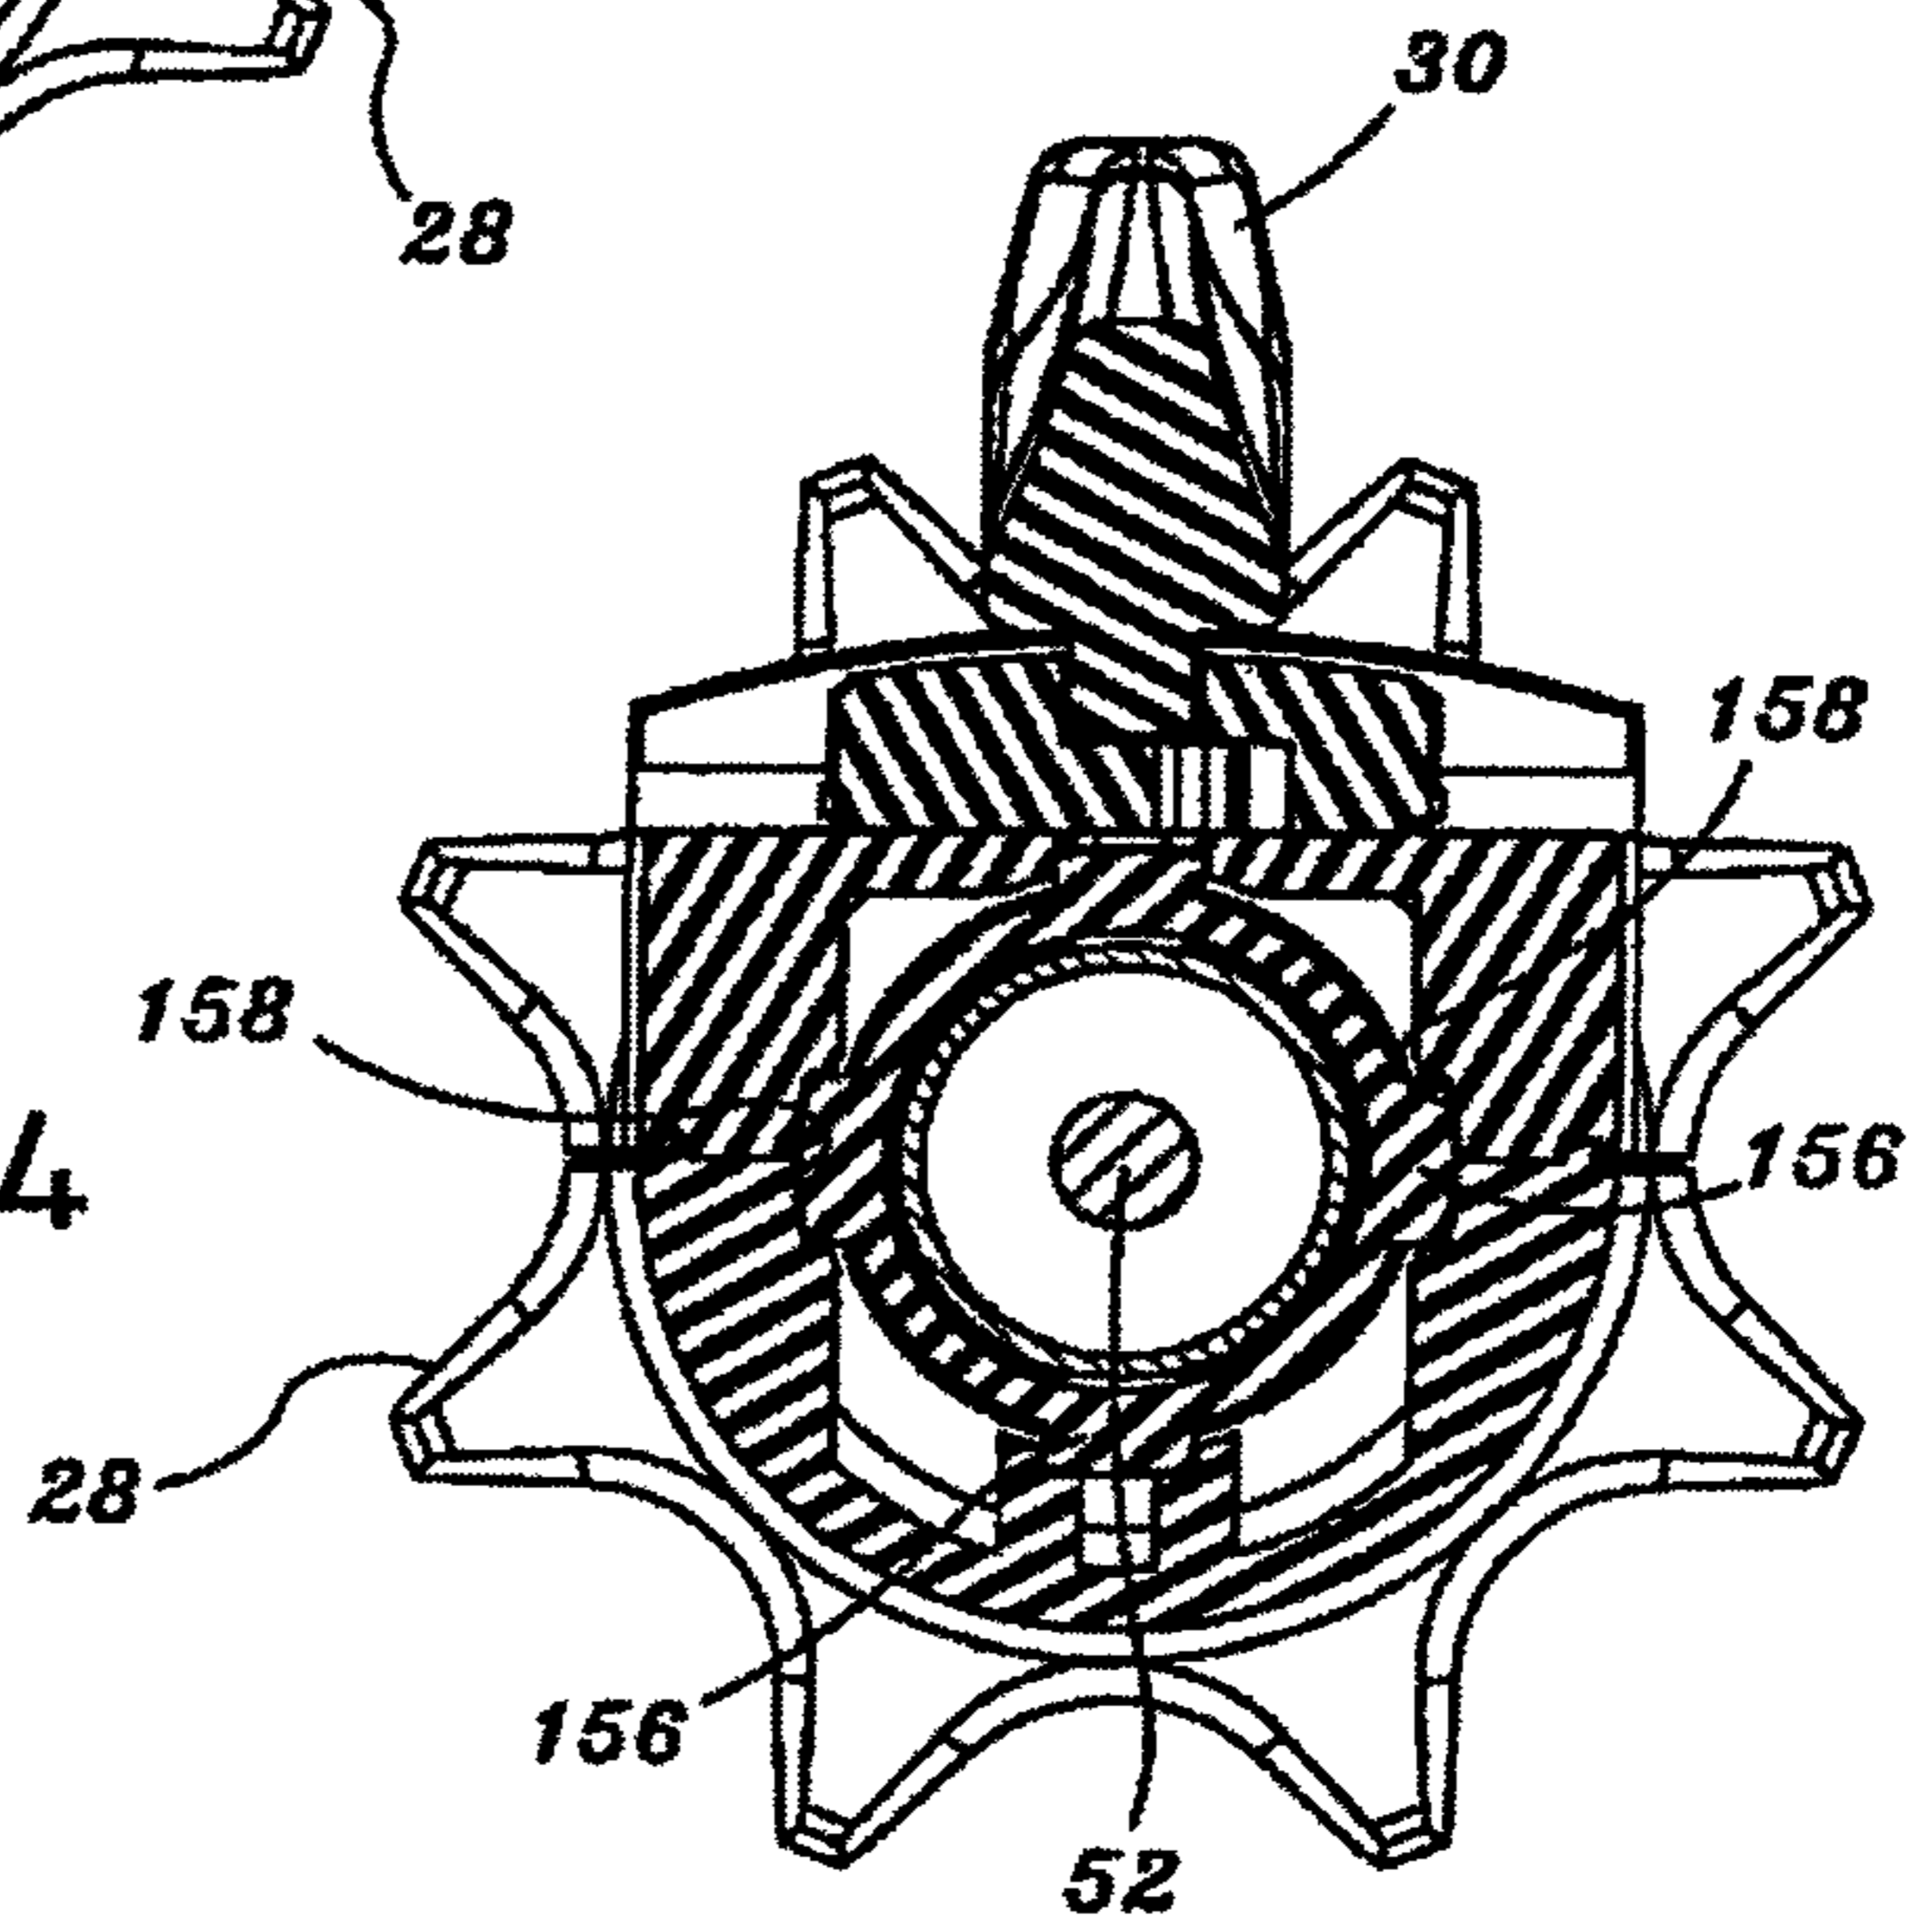


FIG. 14

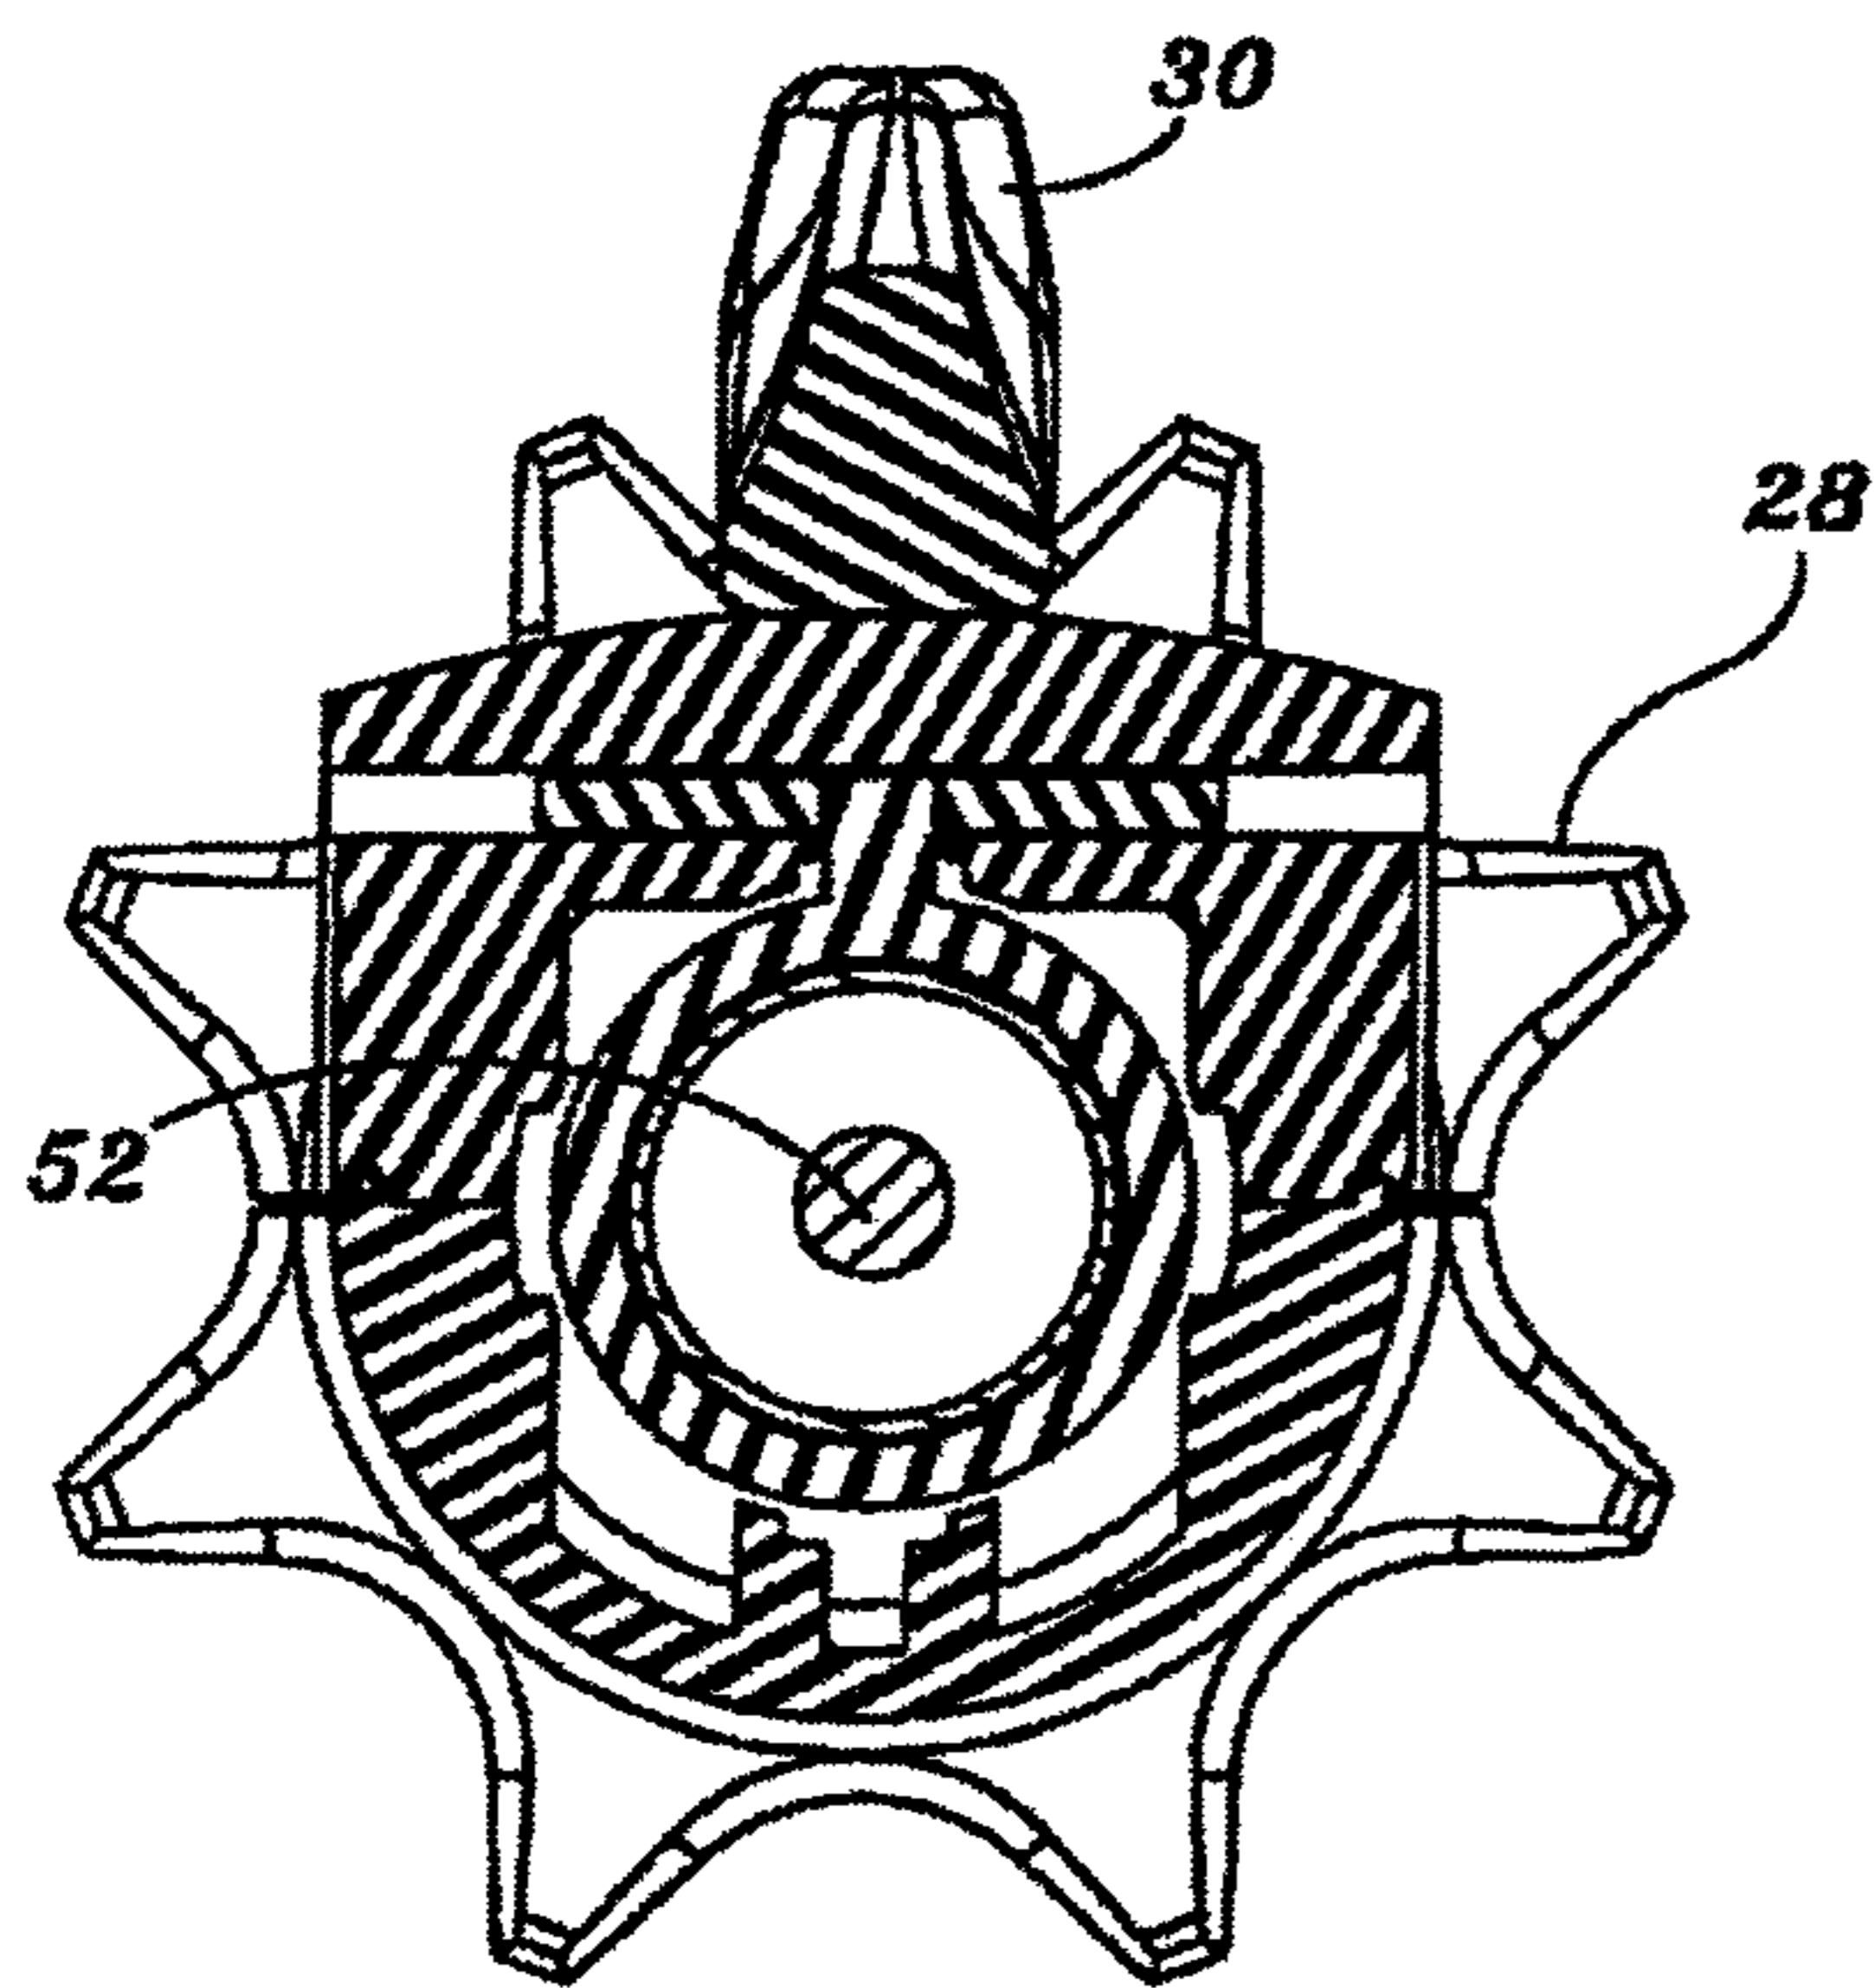


FIG. 15

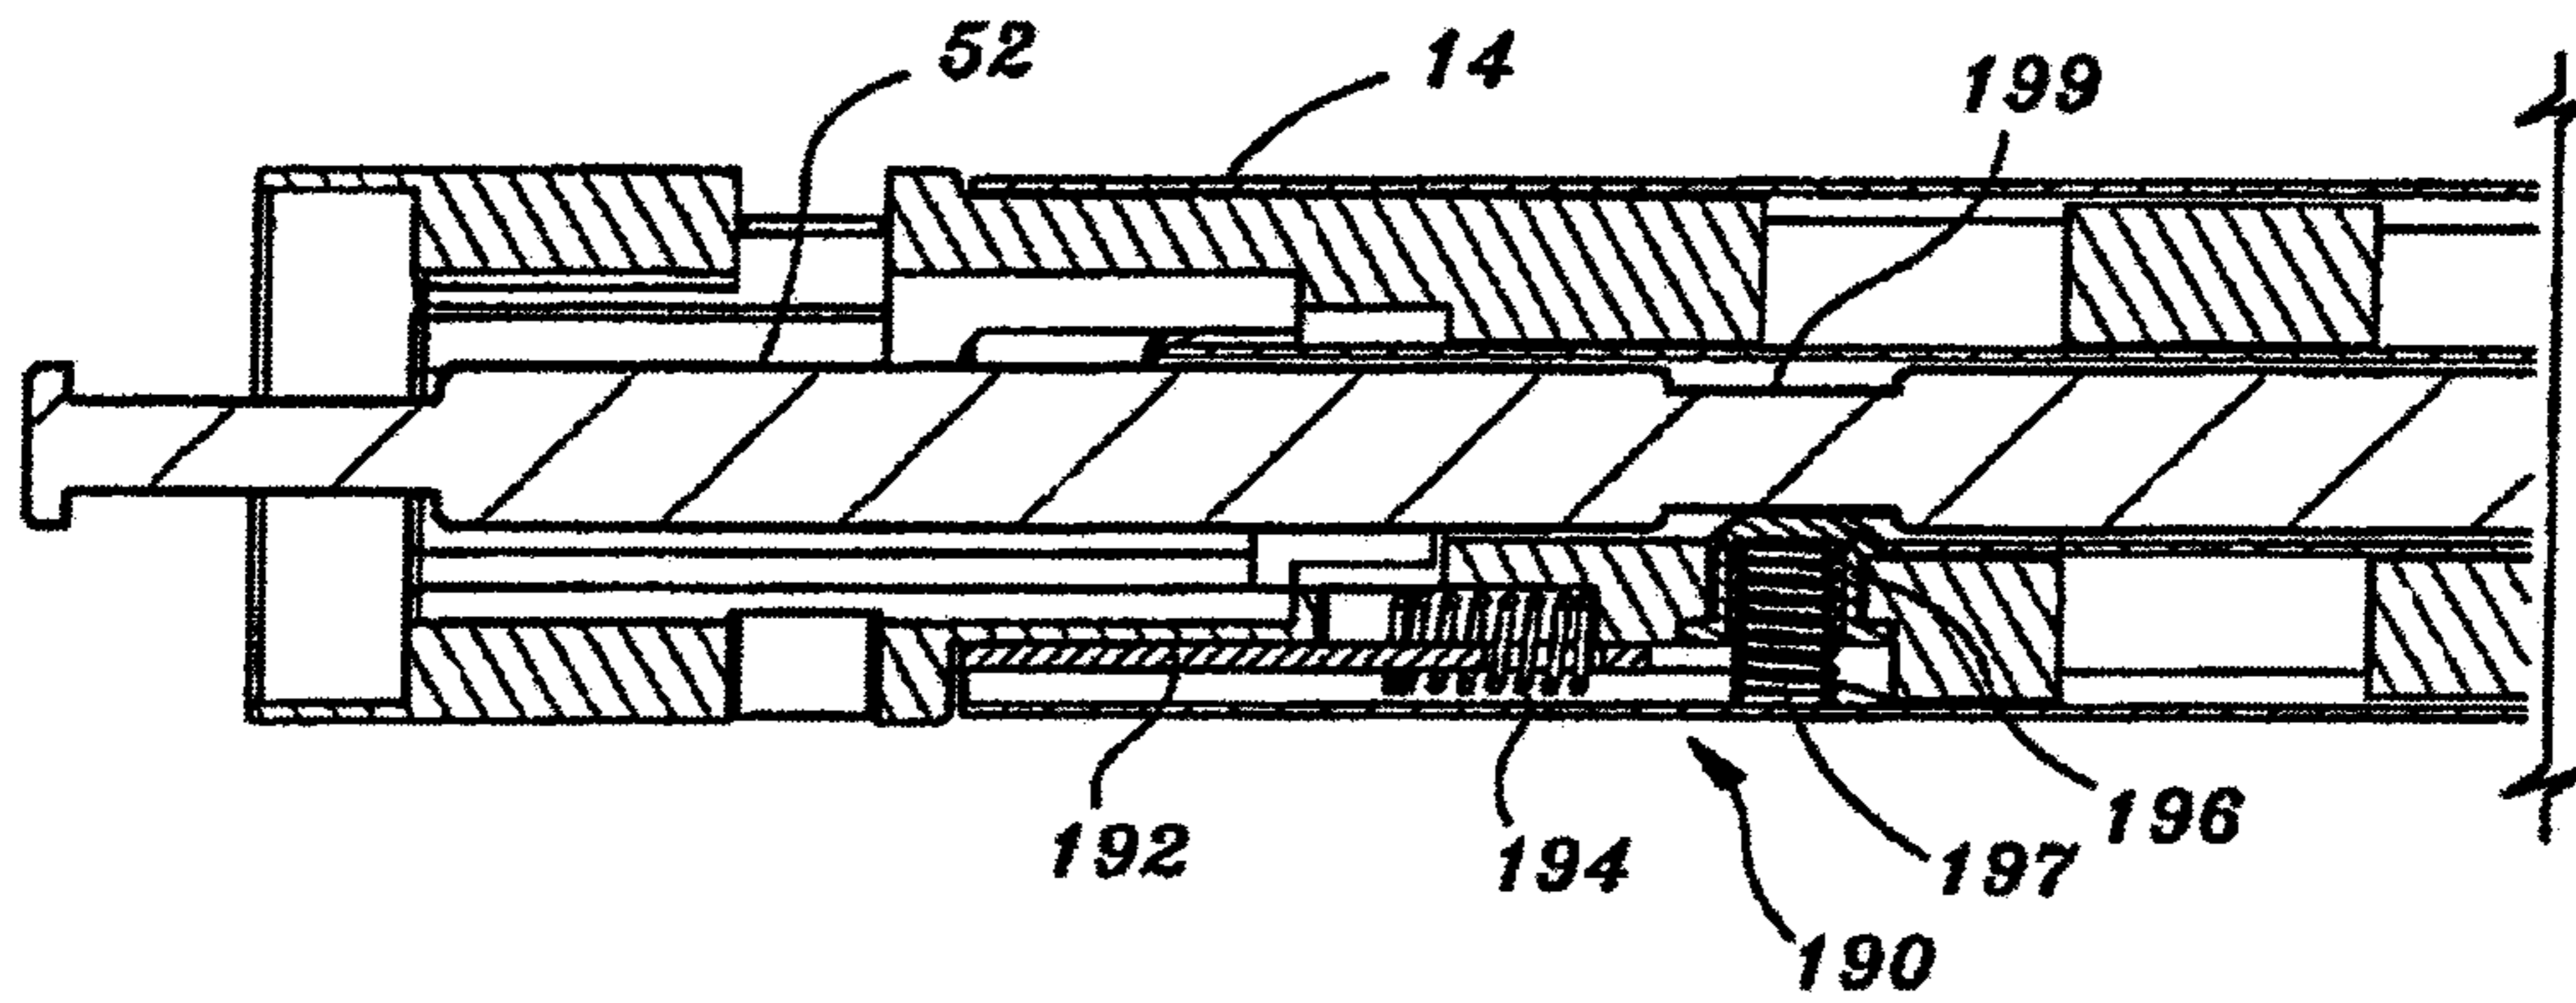


FIG. 16

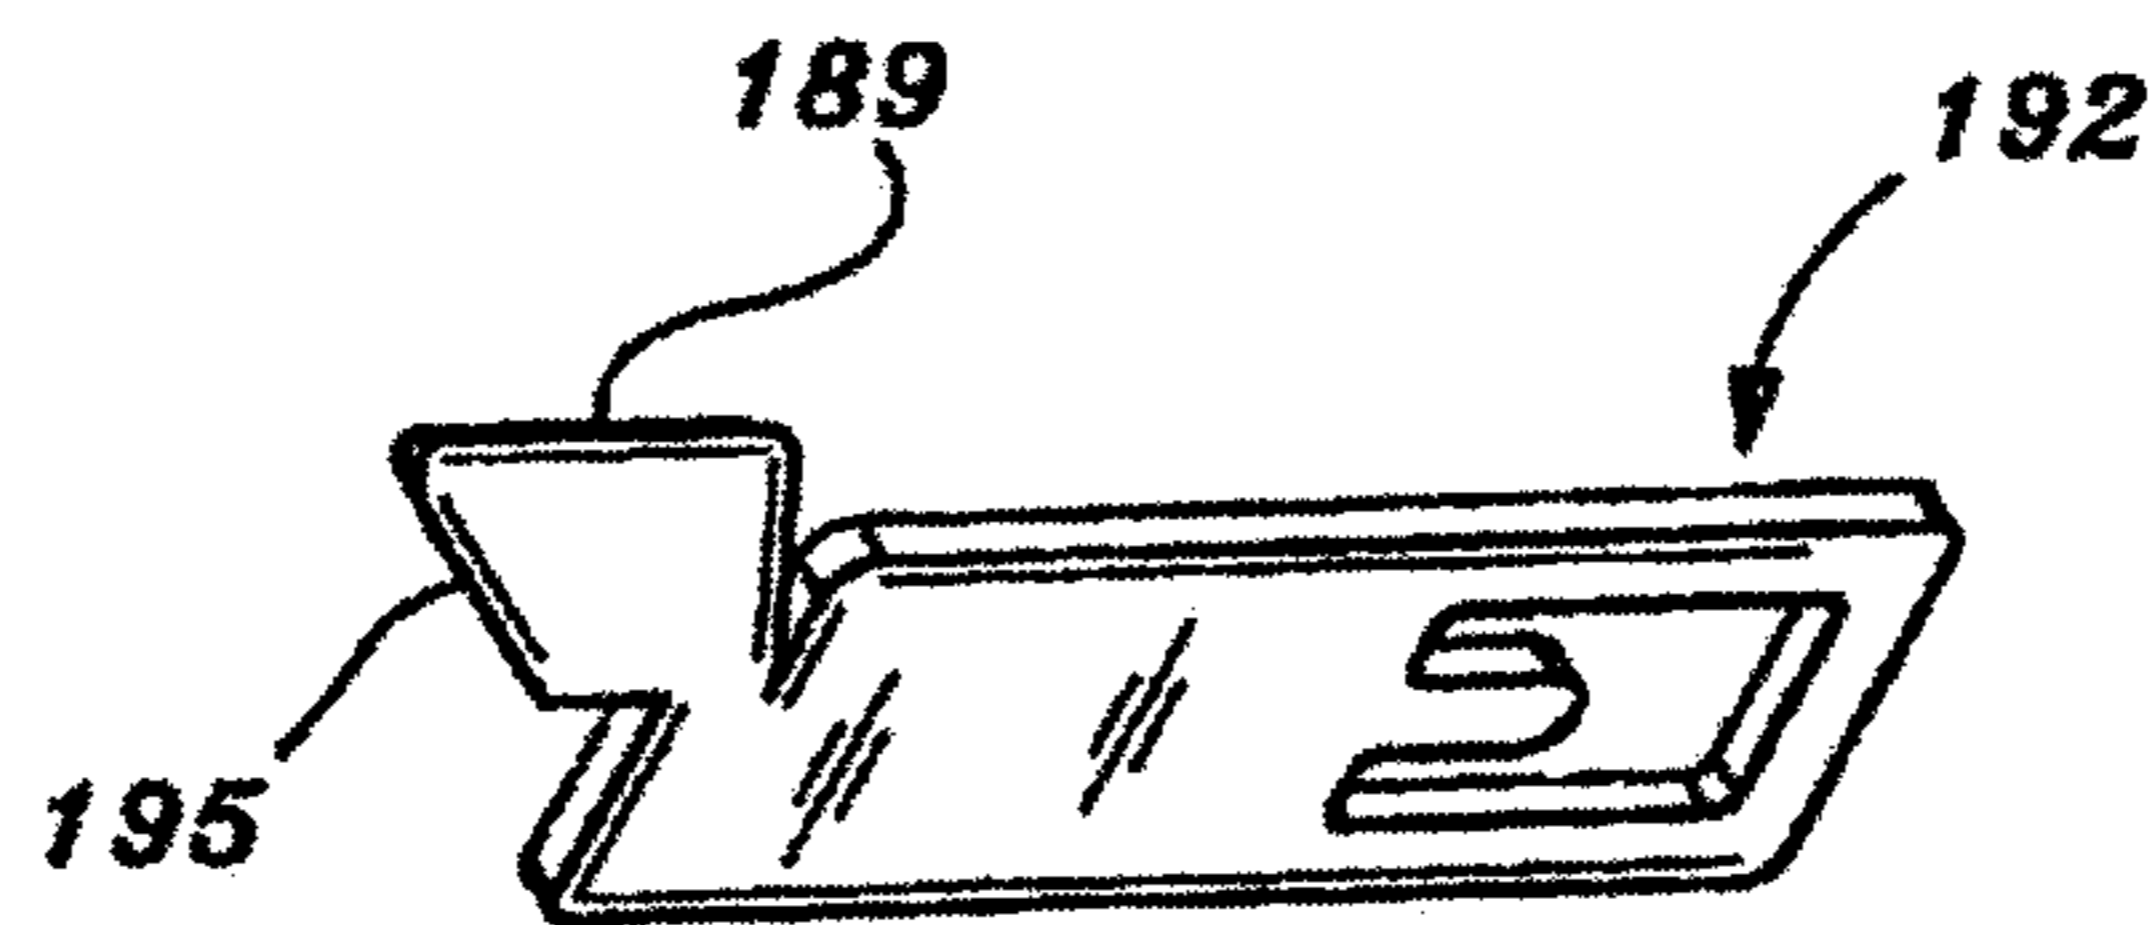


FIG. 17

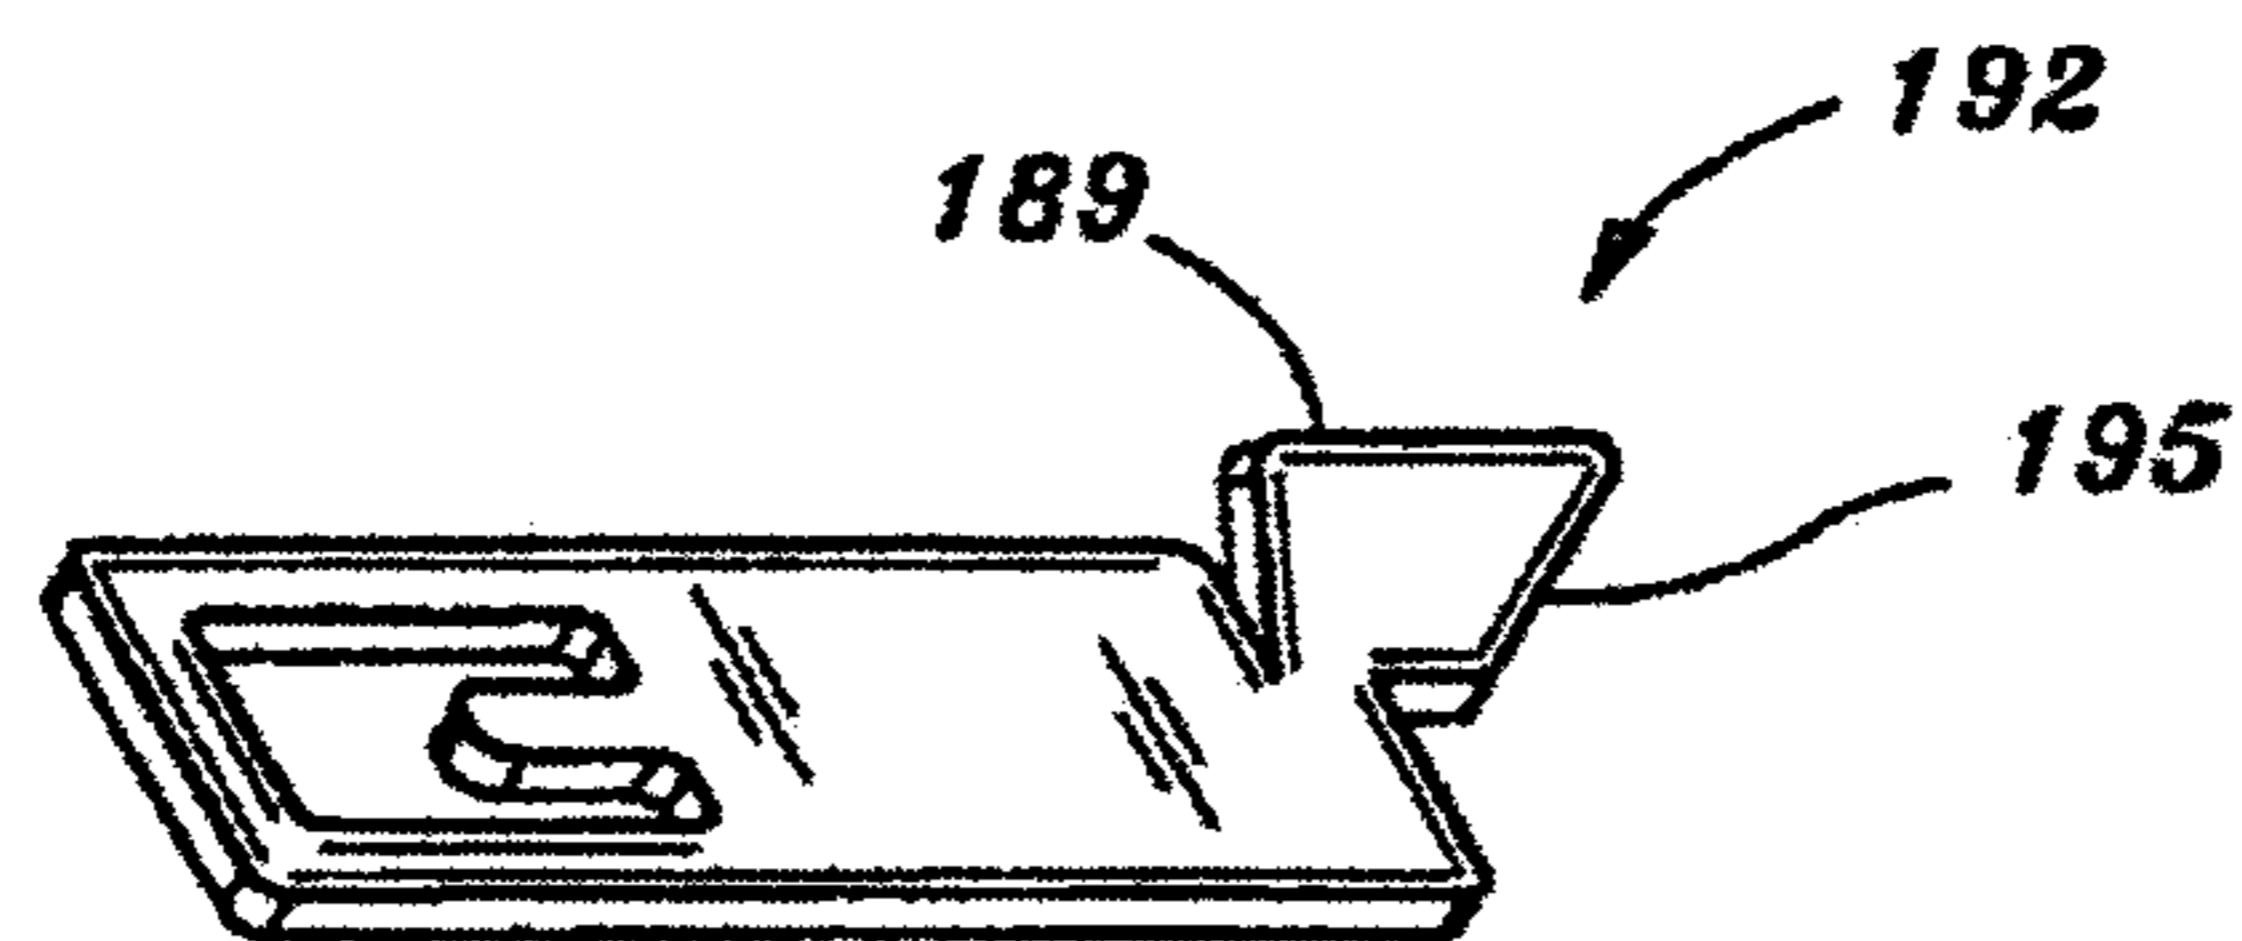


FIG. 18

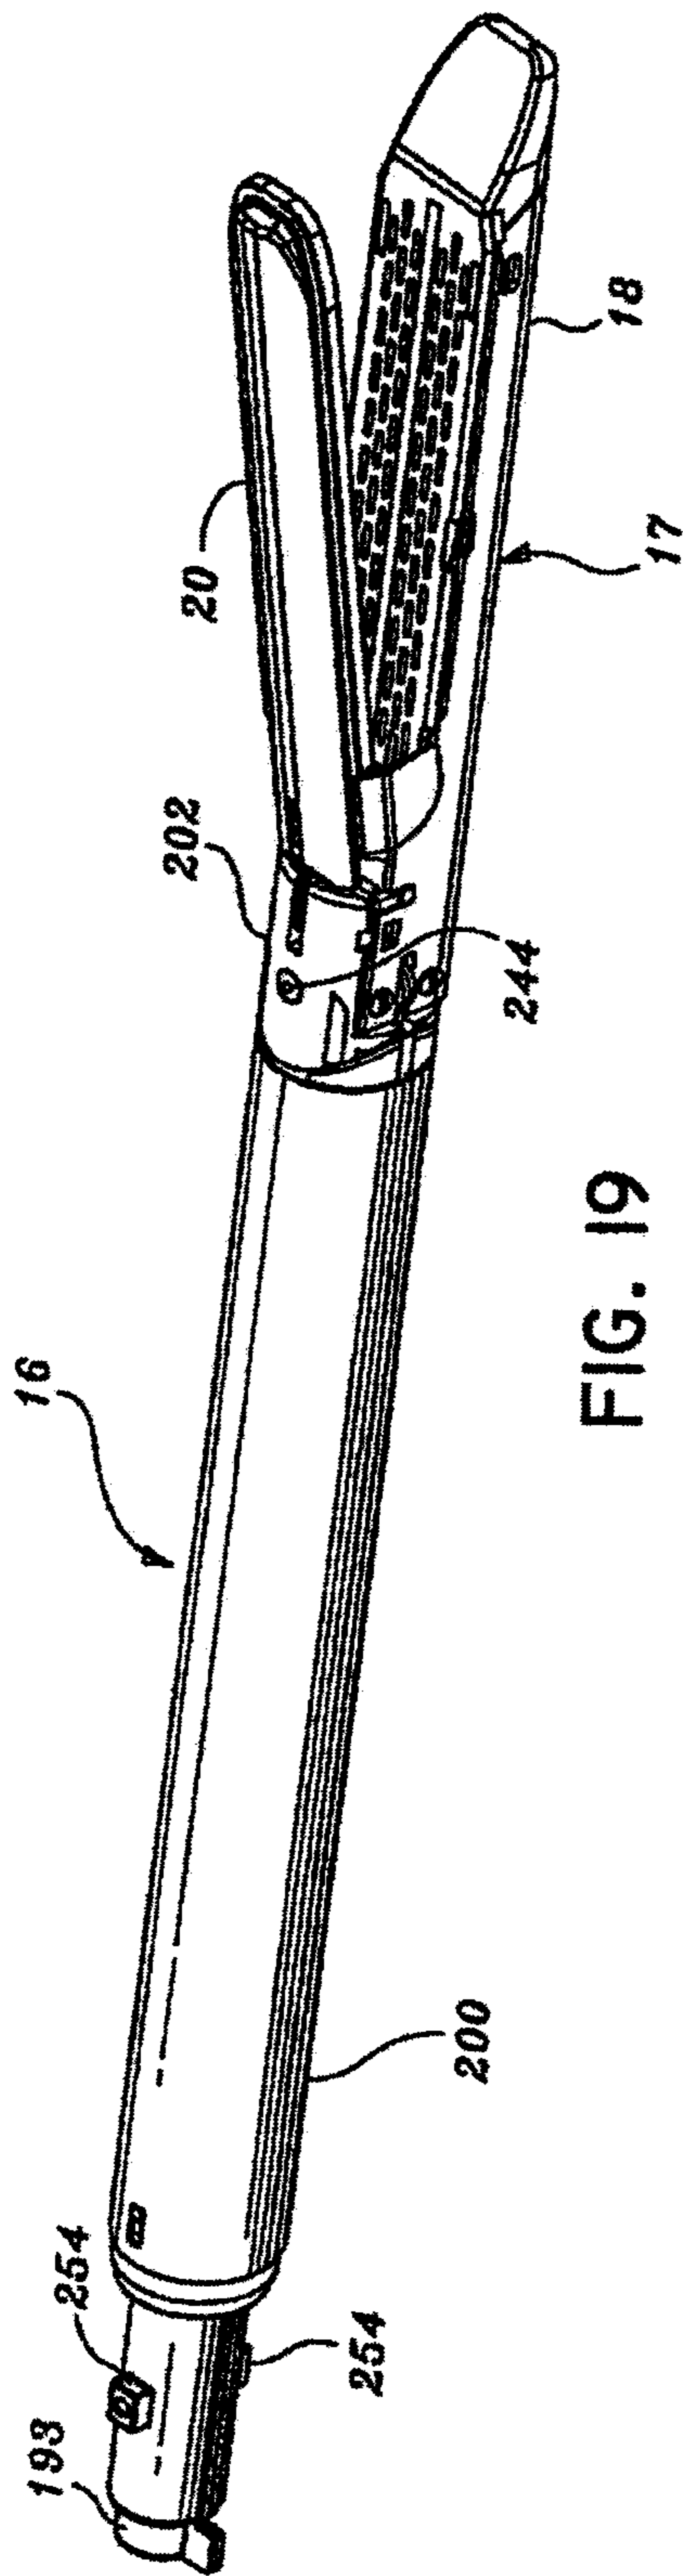


FIG. 19

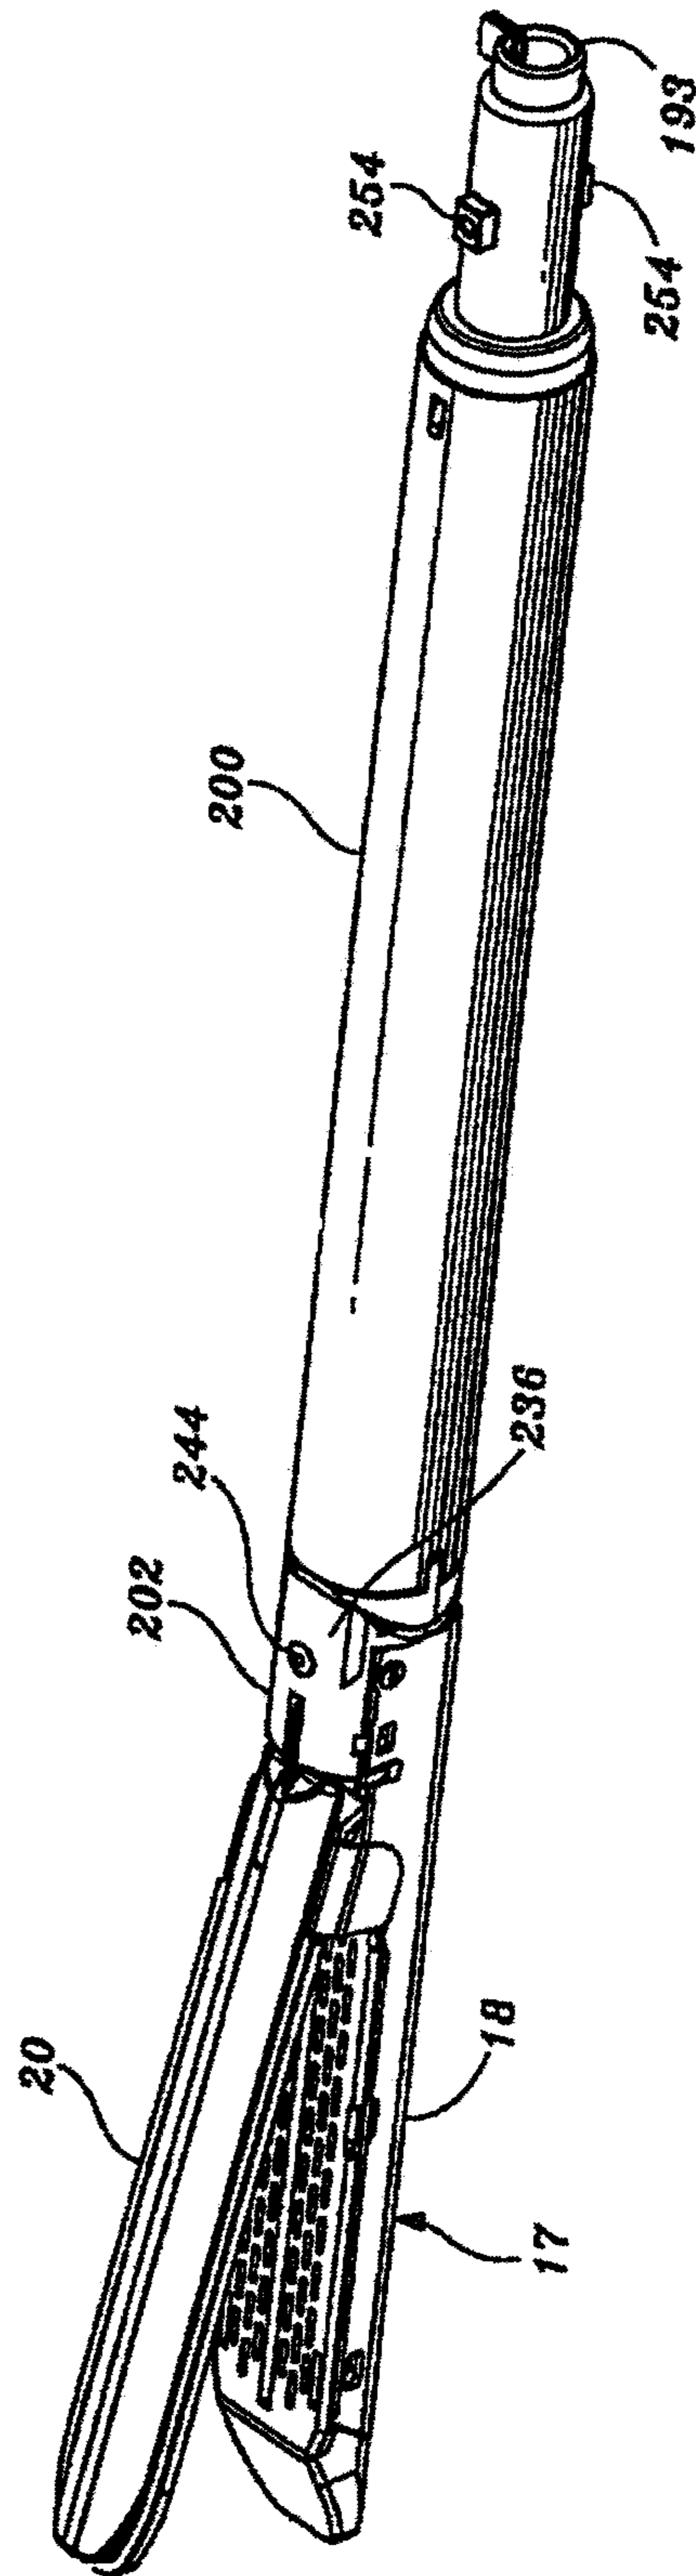


FIG. 20

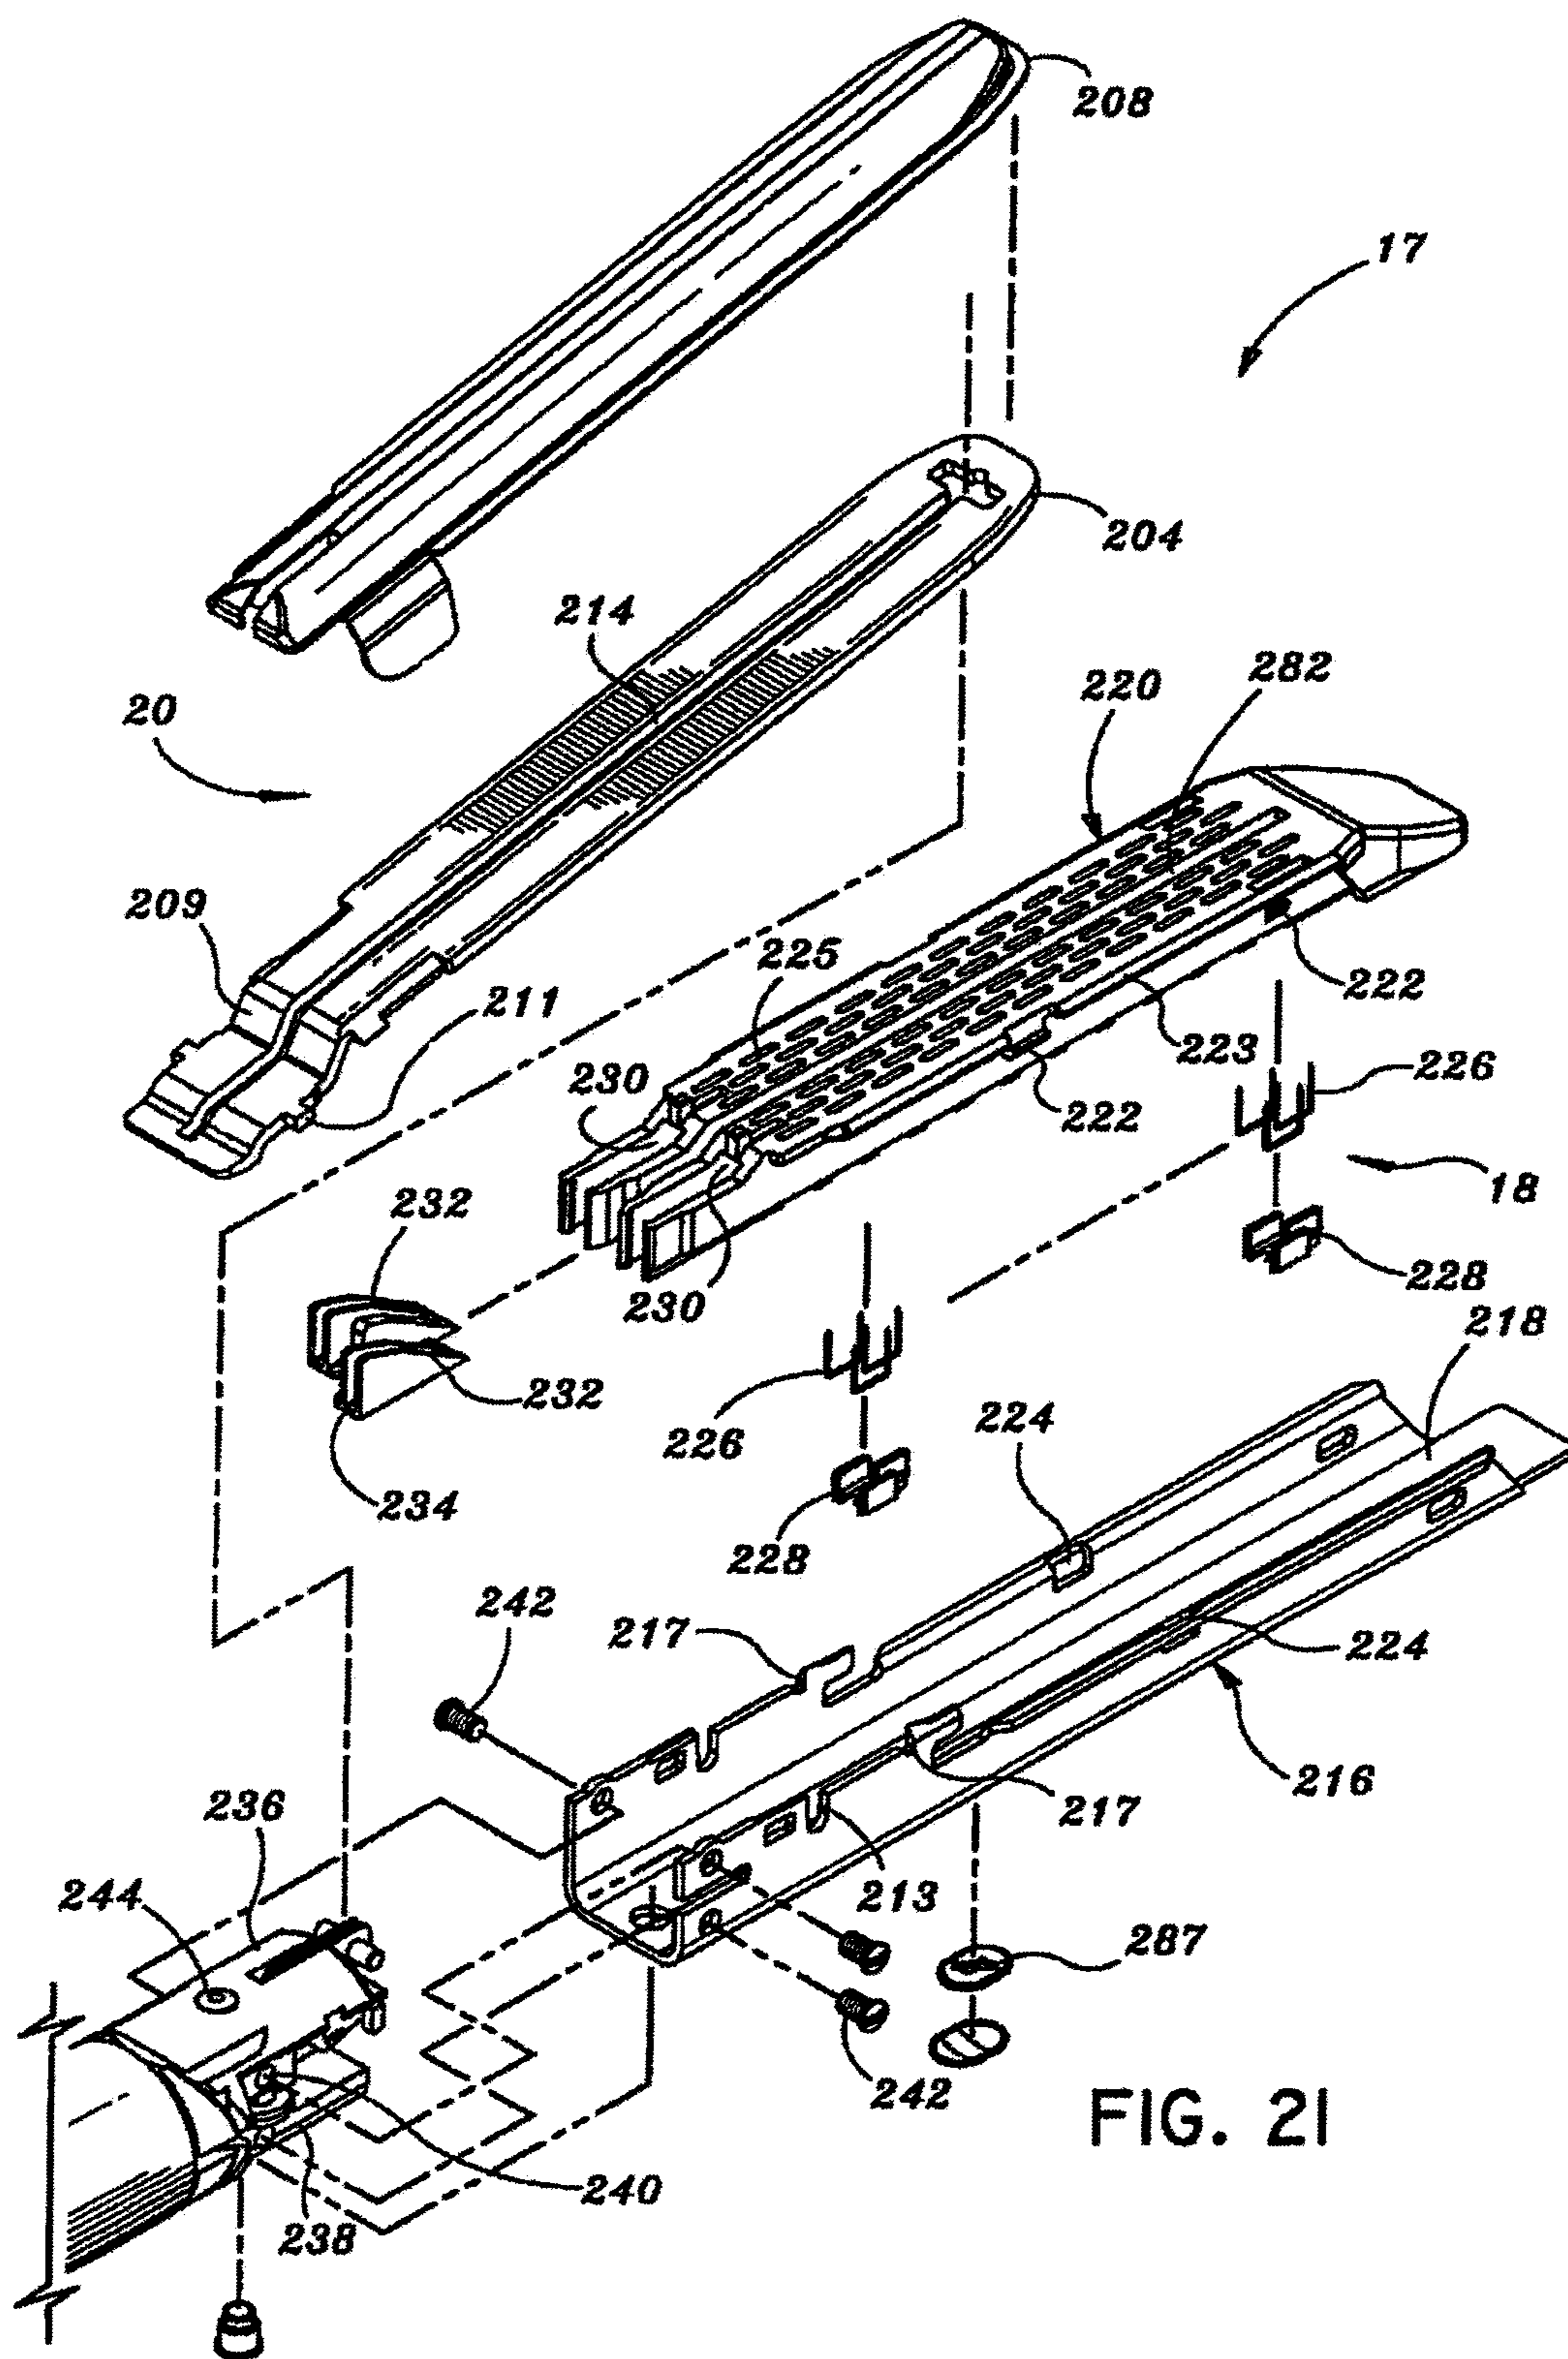


FIG. 21

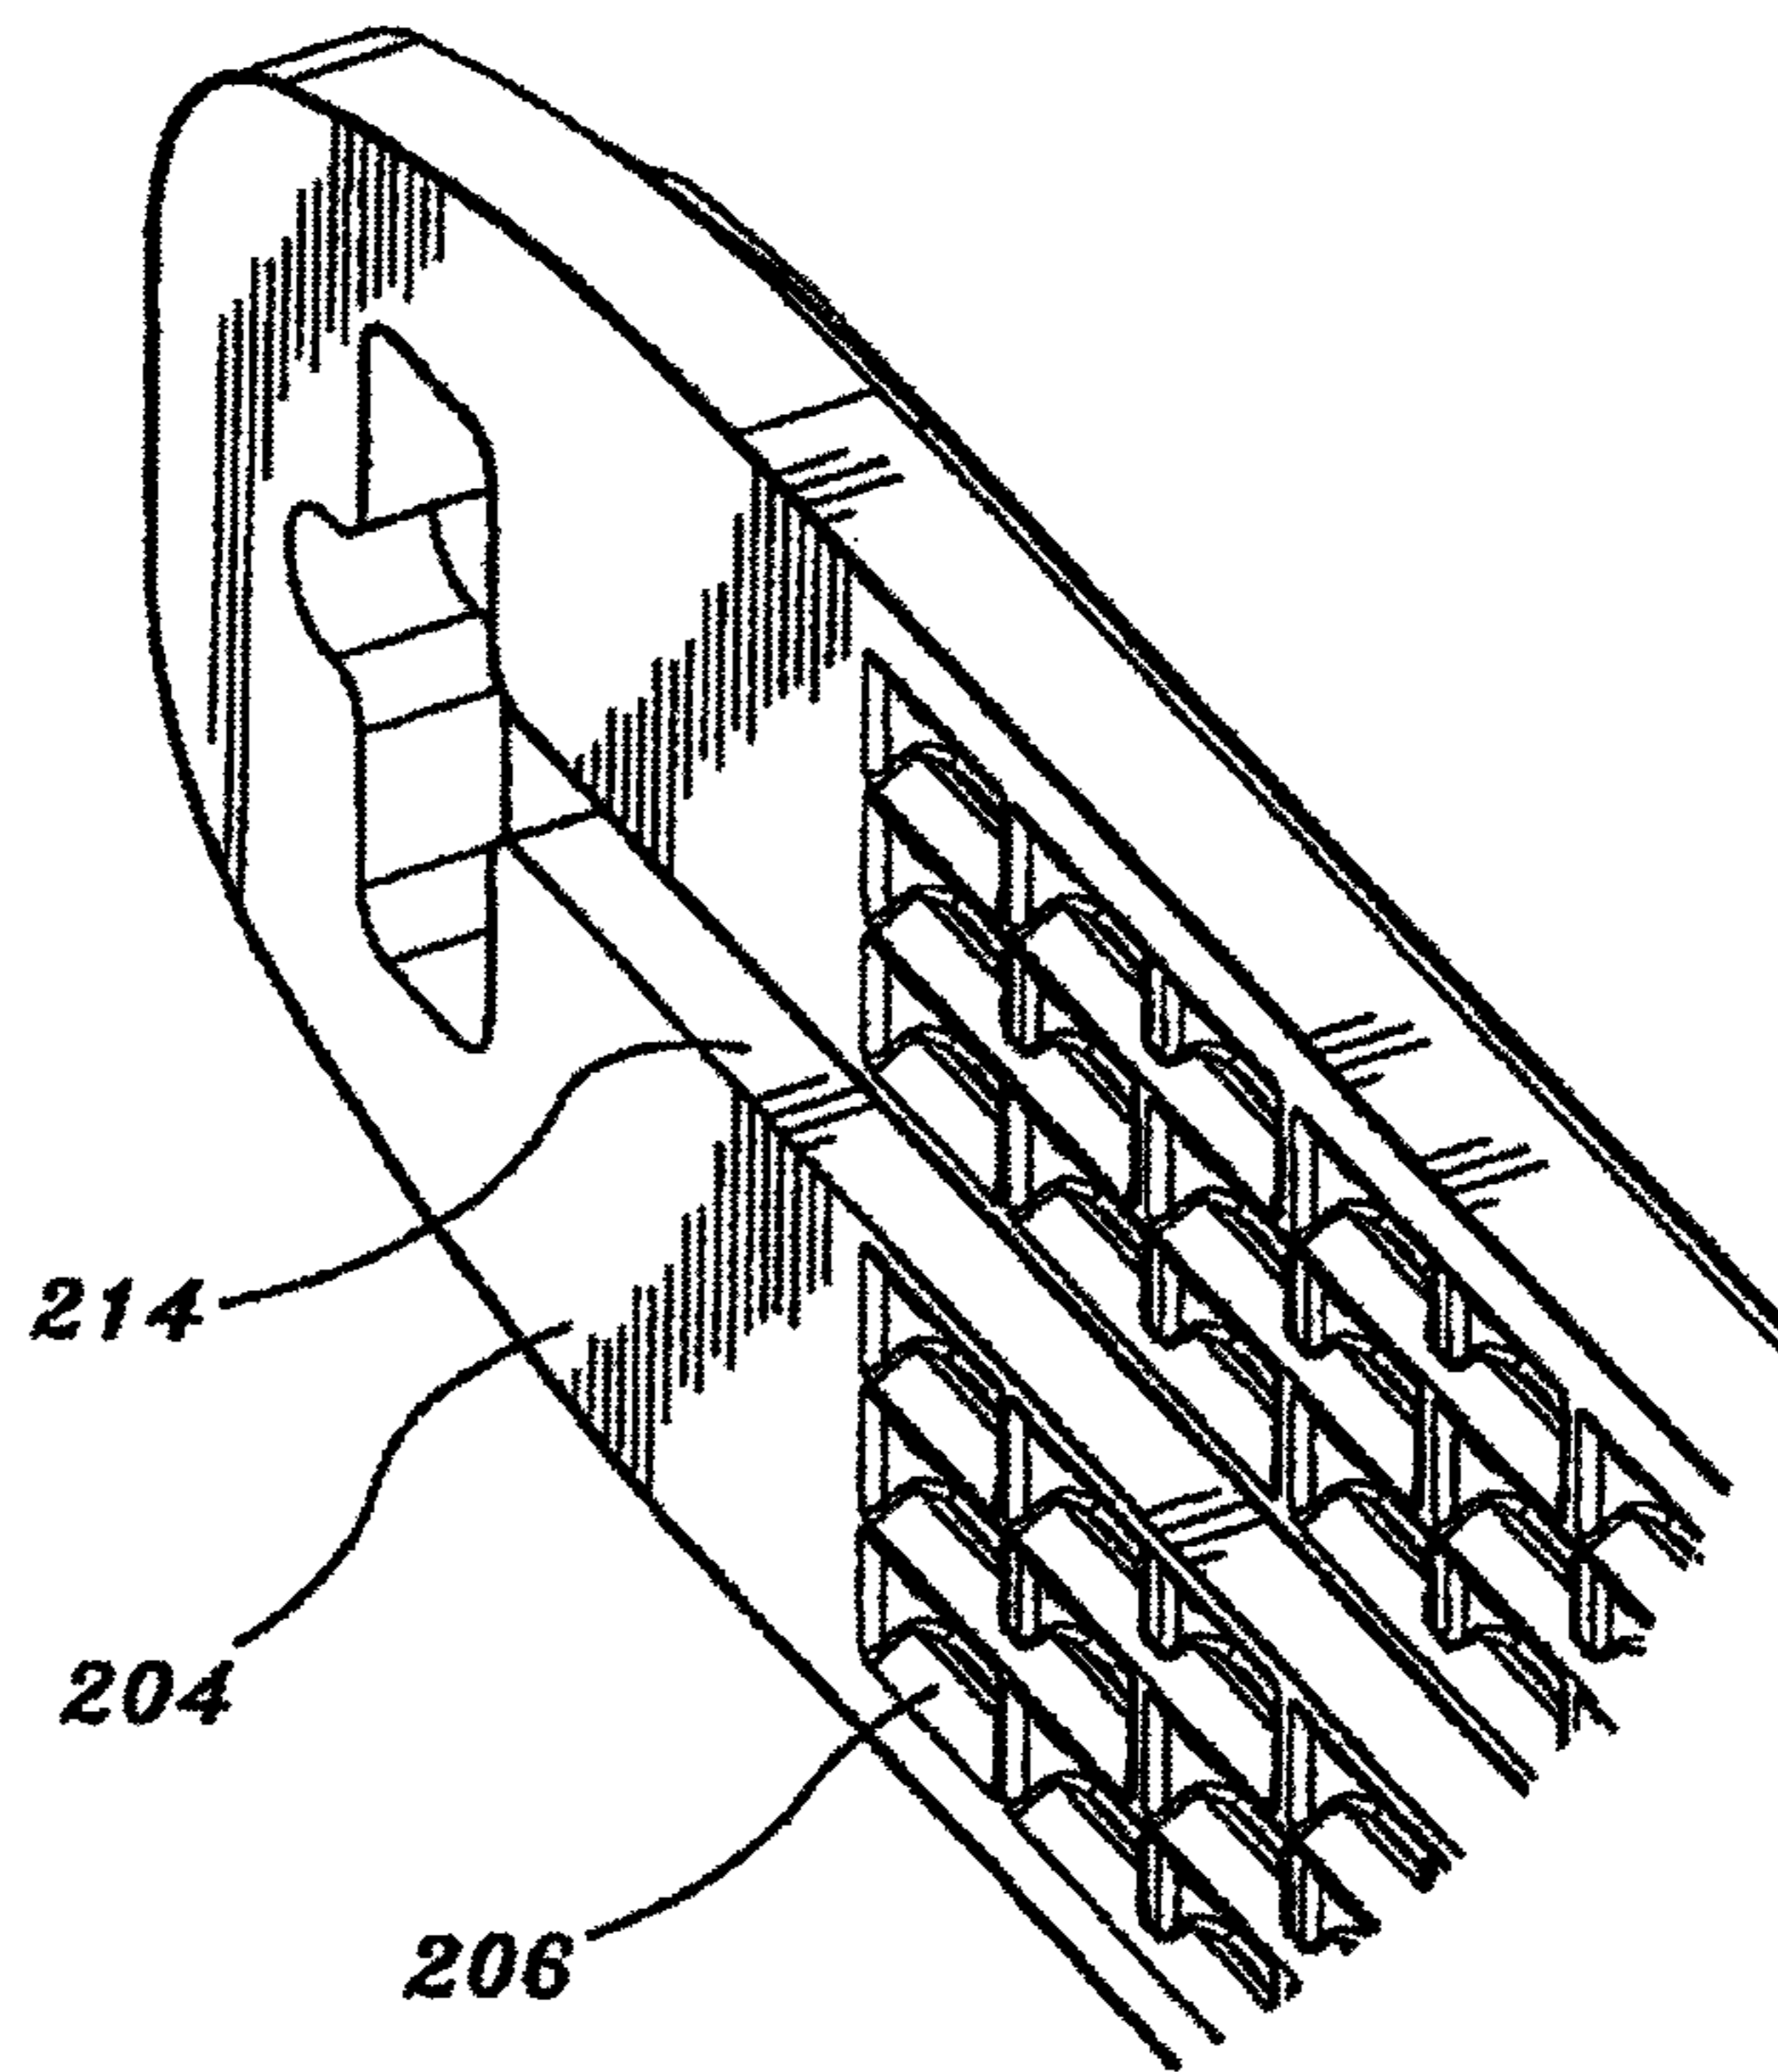


FIG. 22



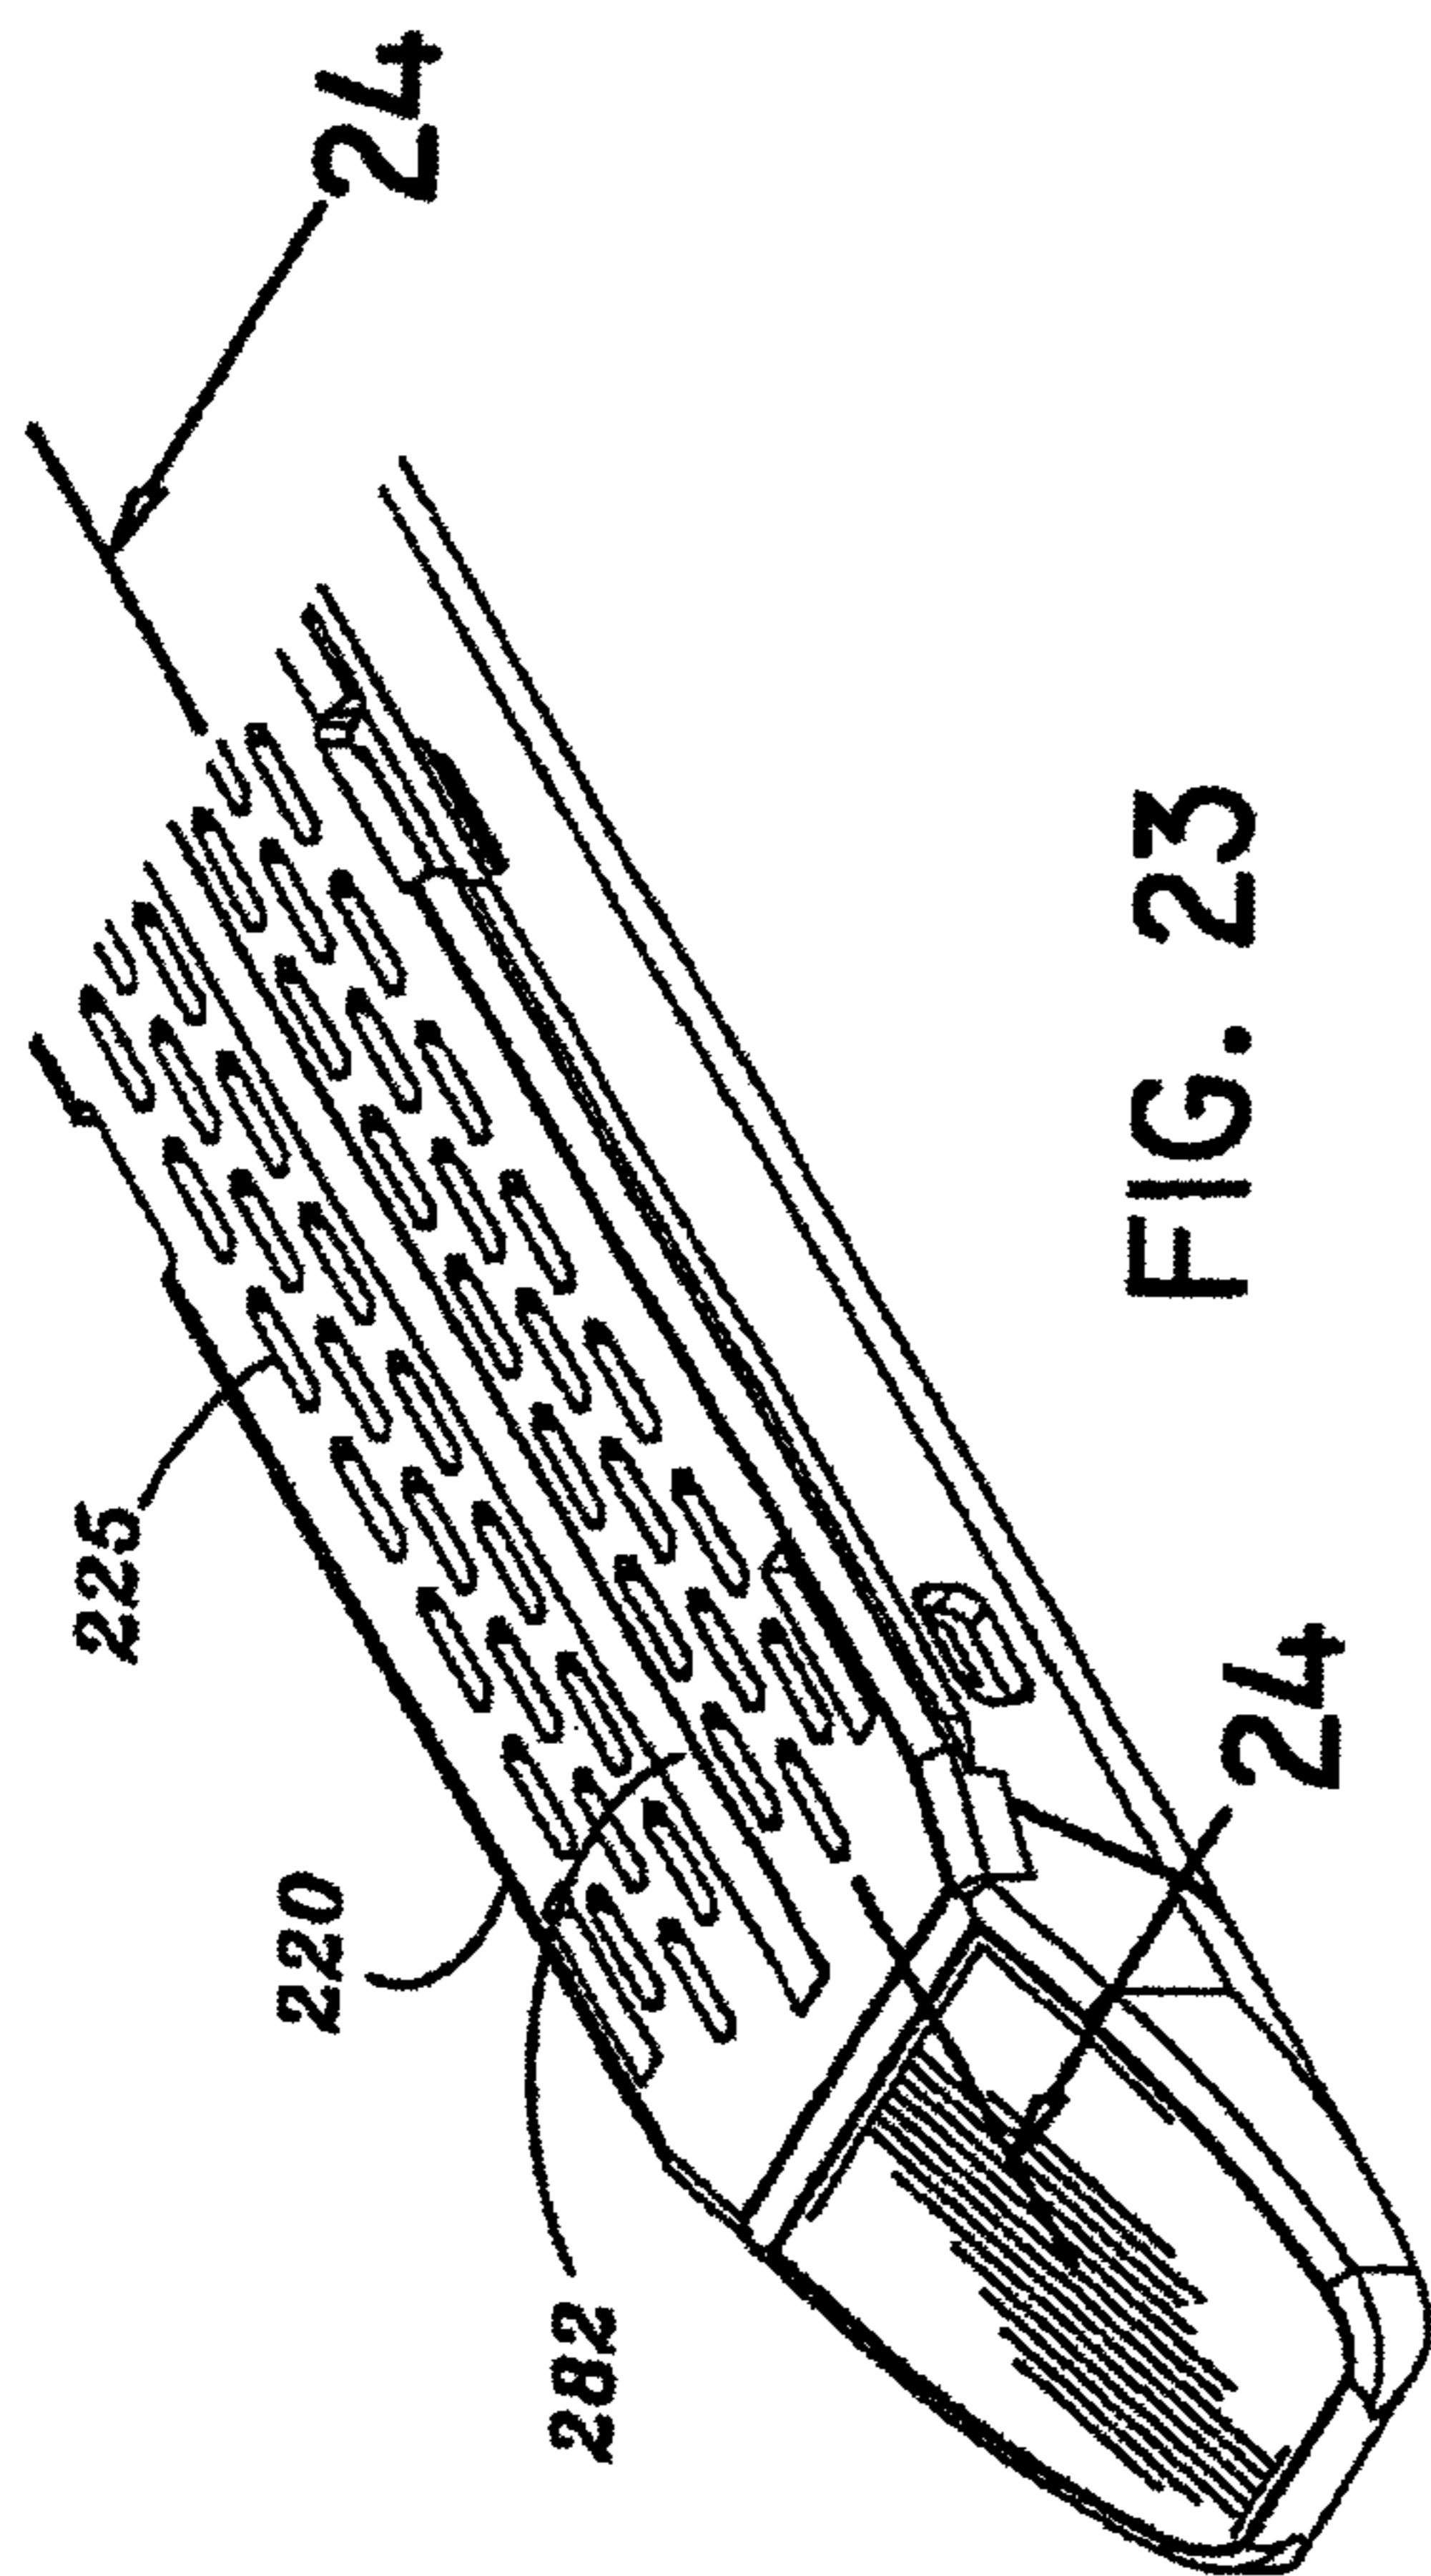


FIG. 23

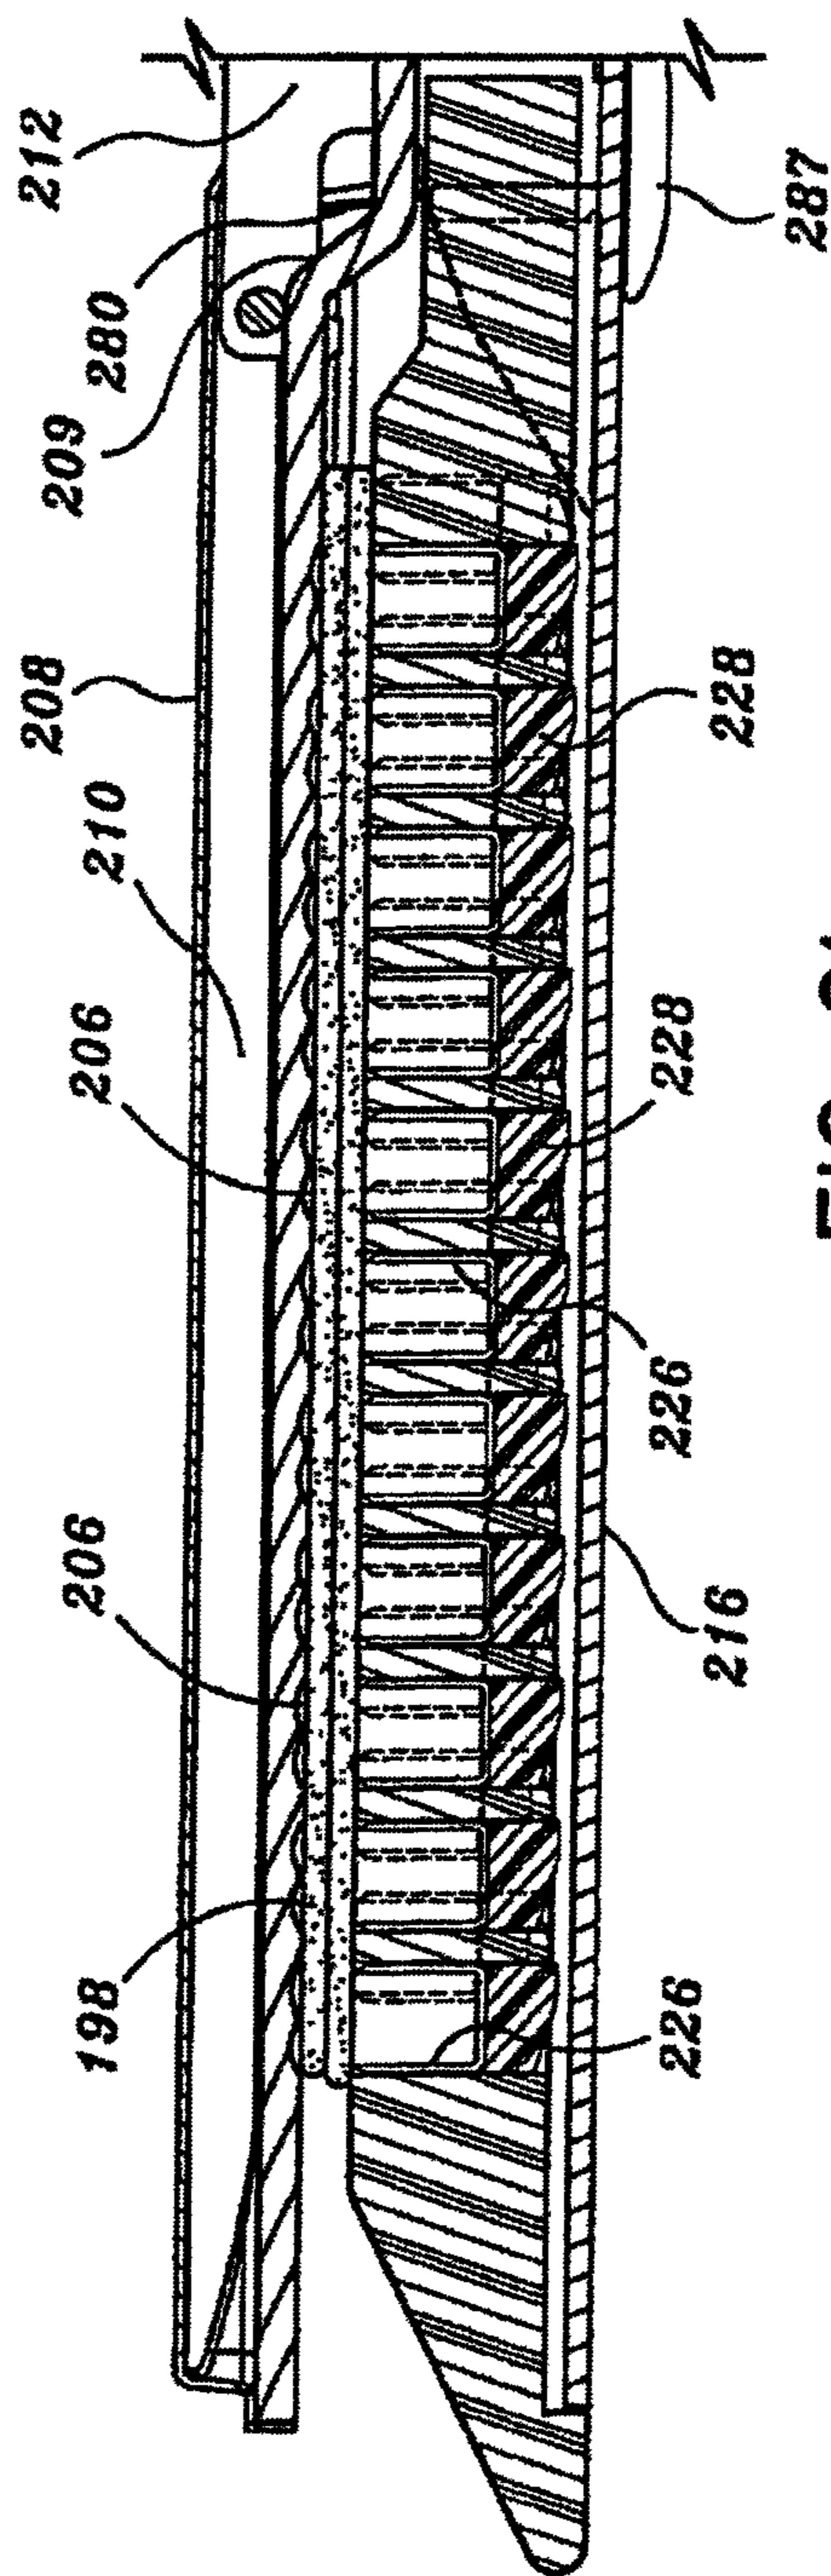


FIG. 24

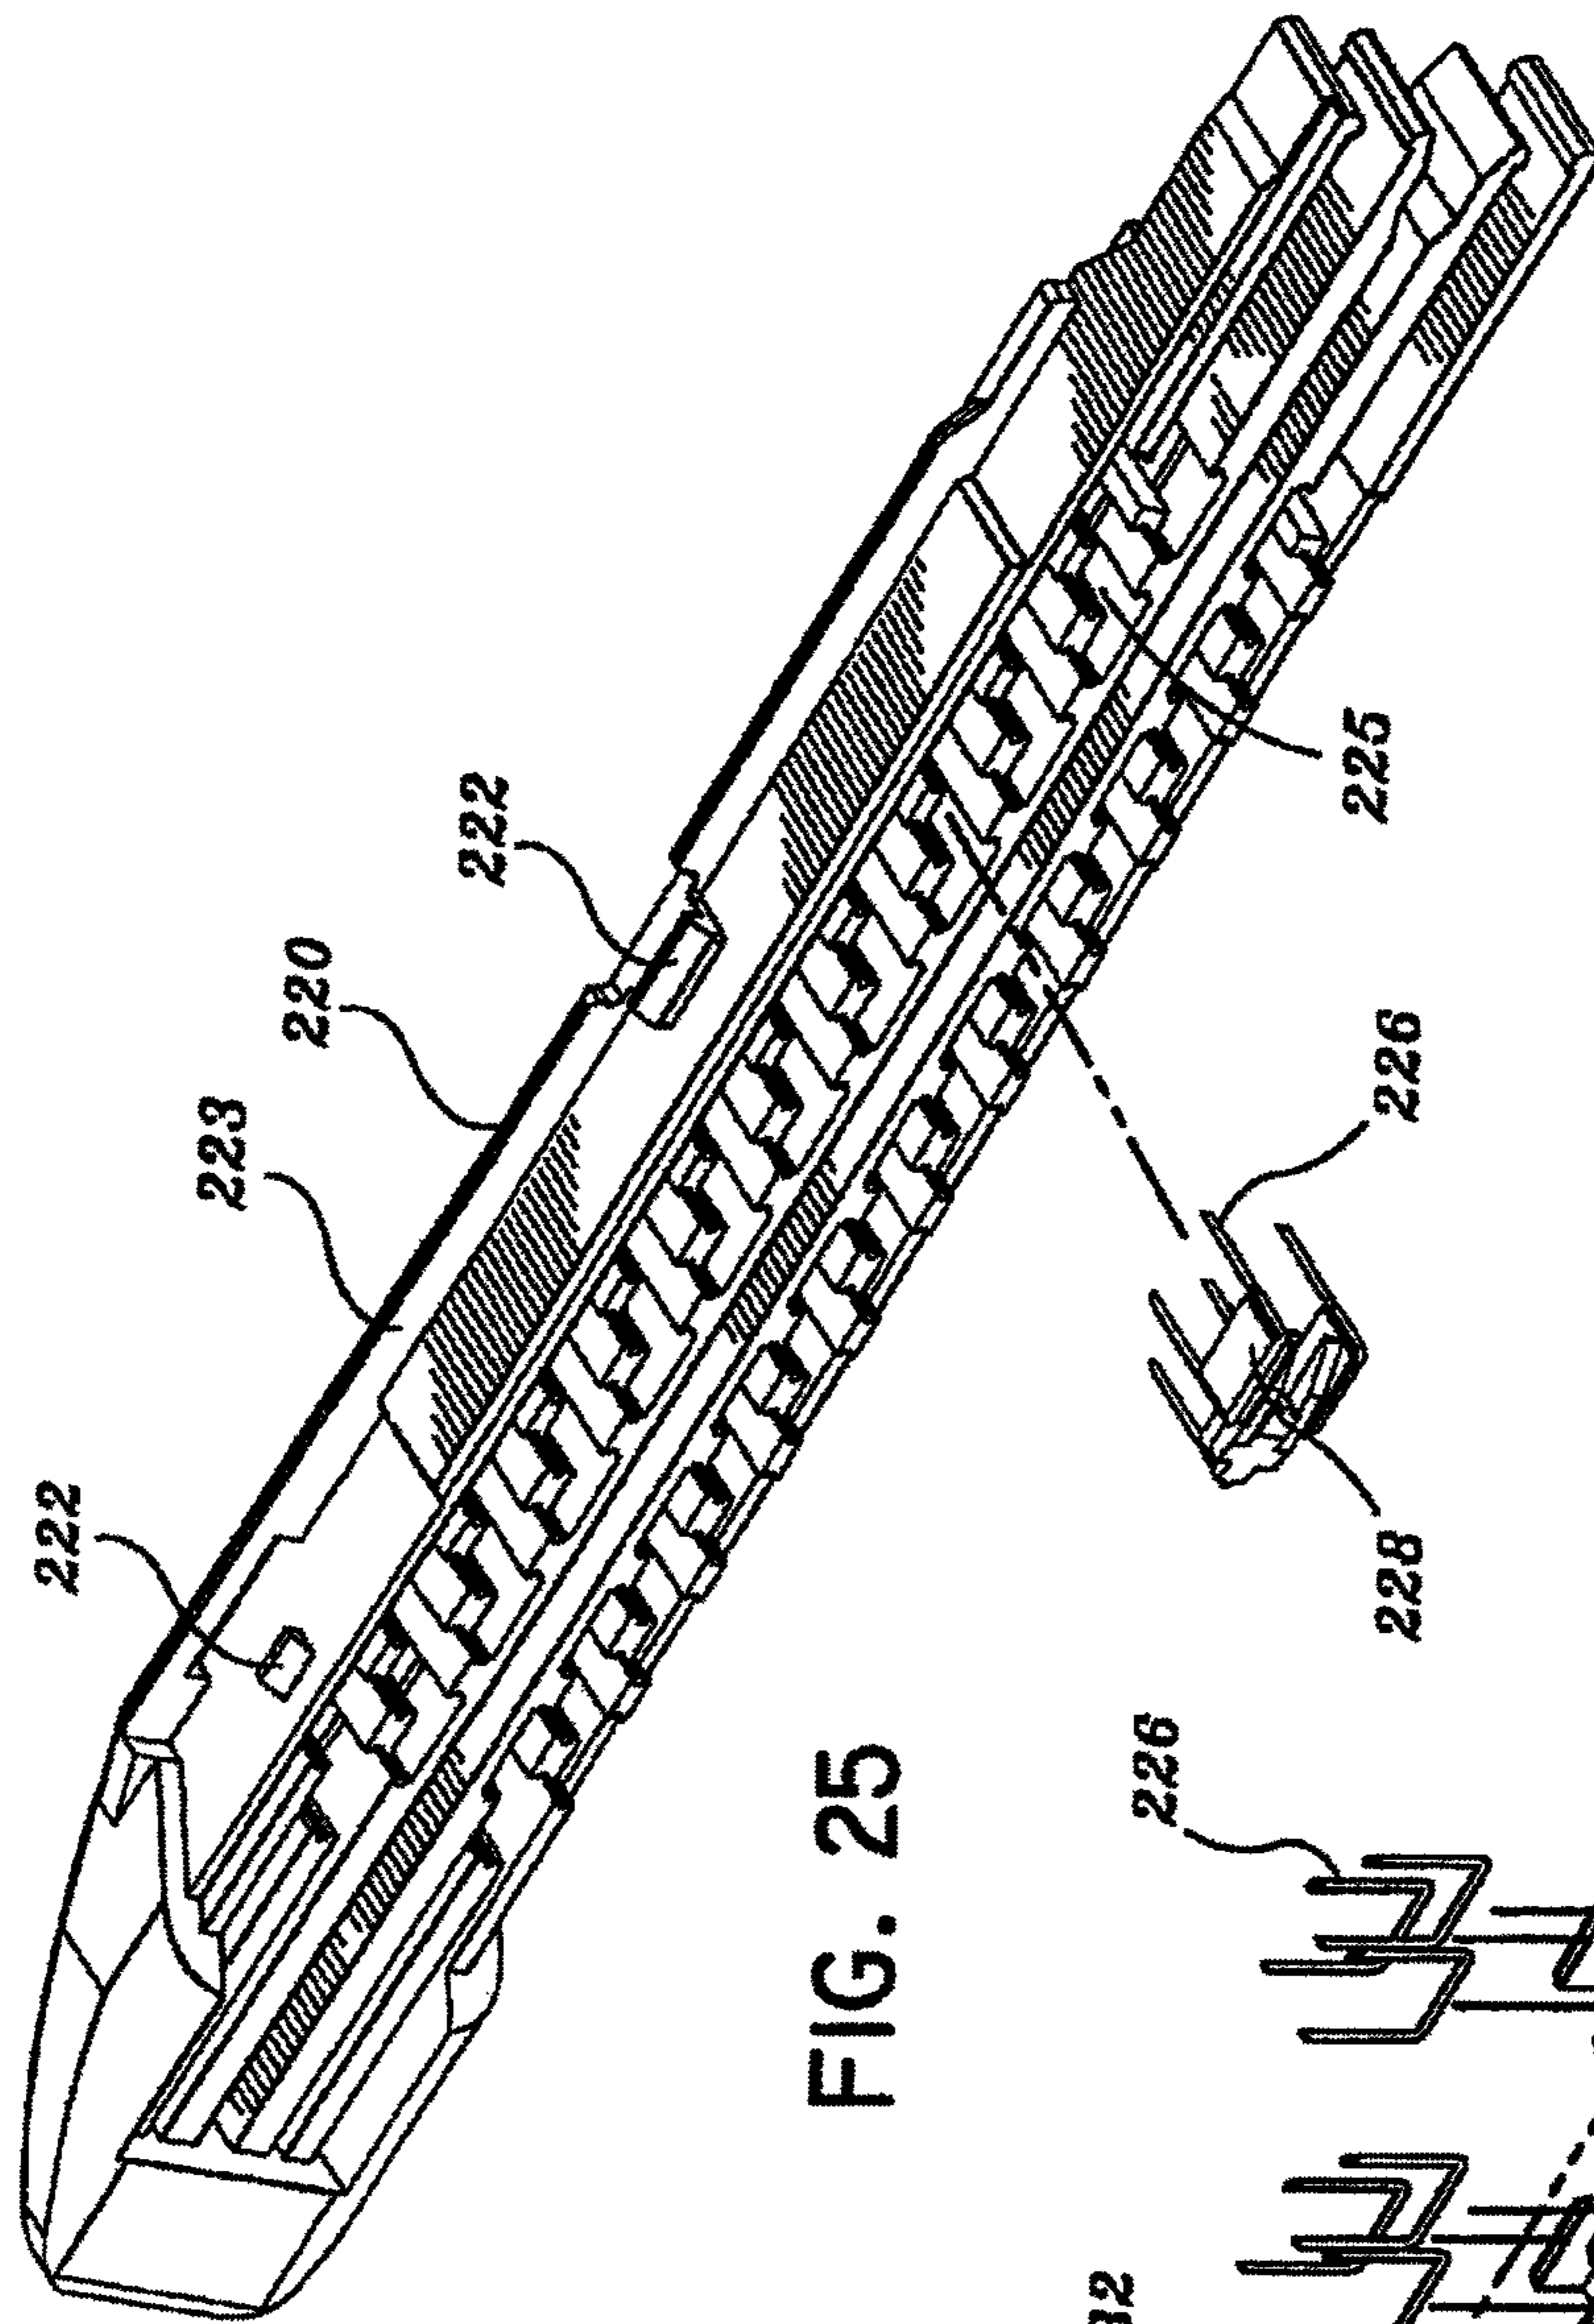


FIG. 25

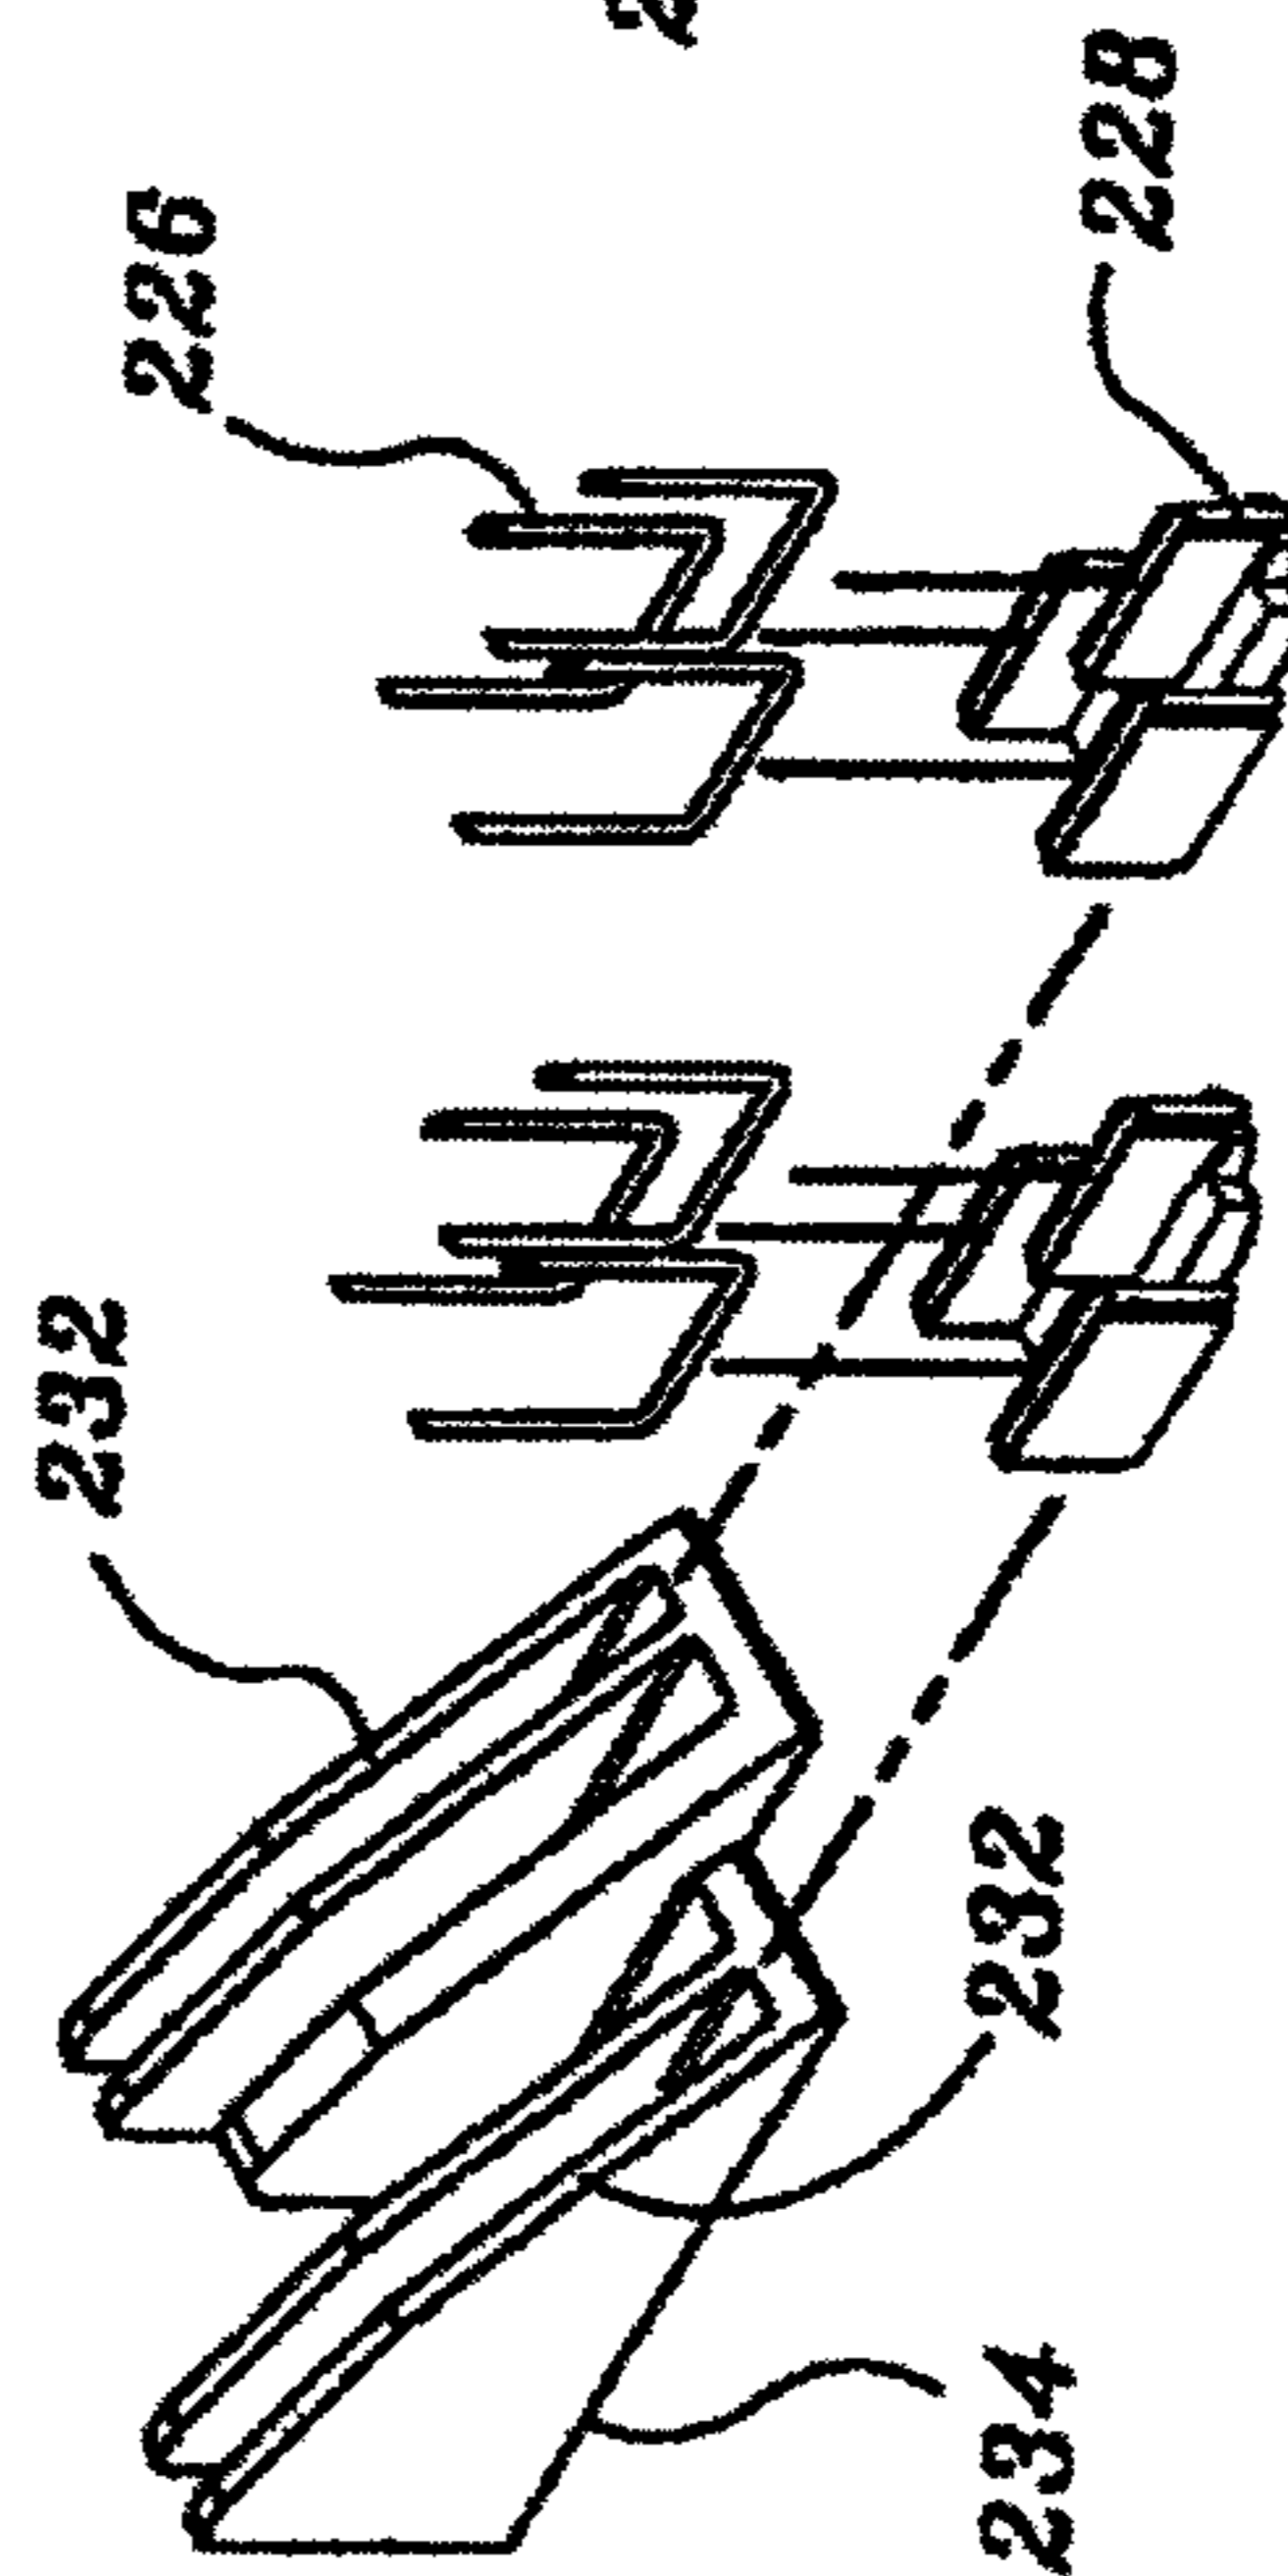
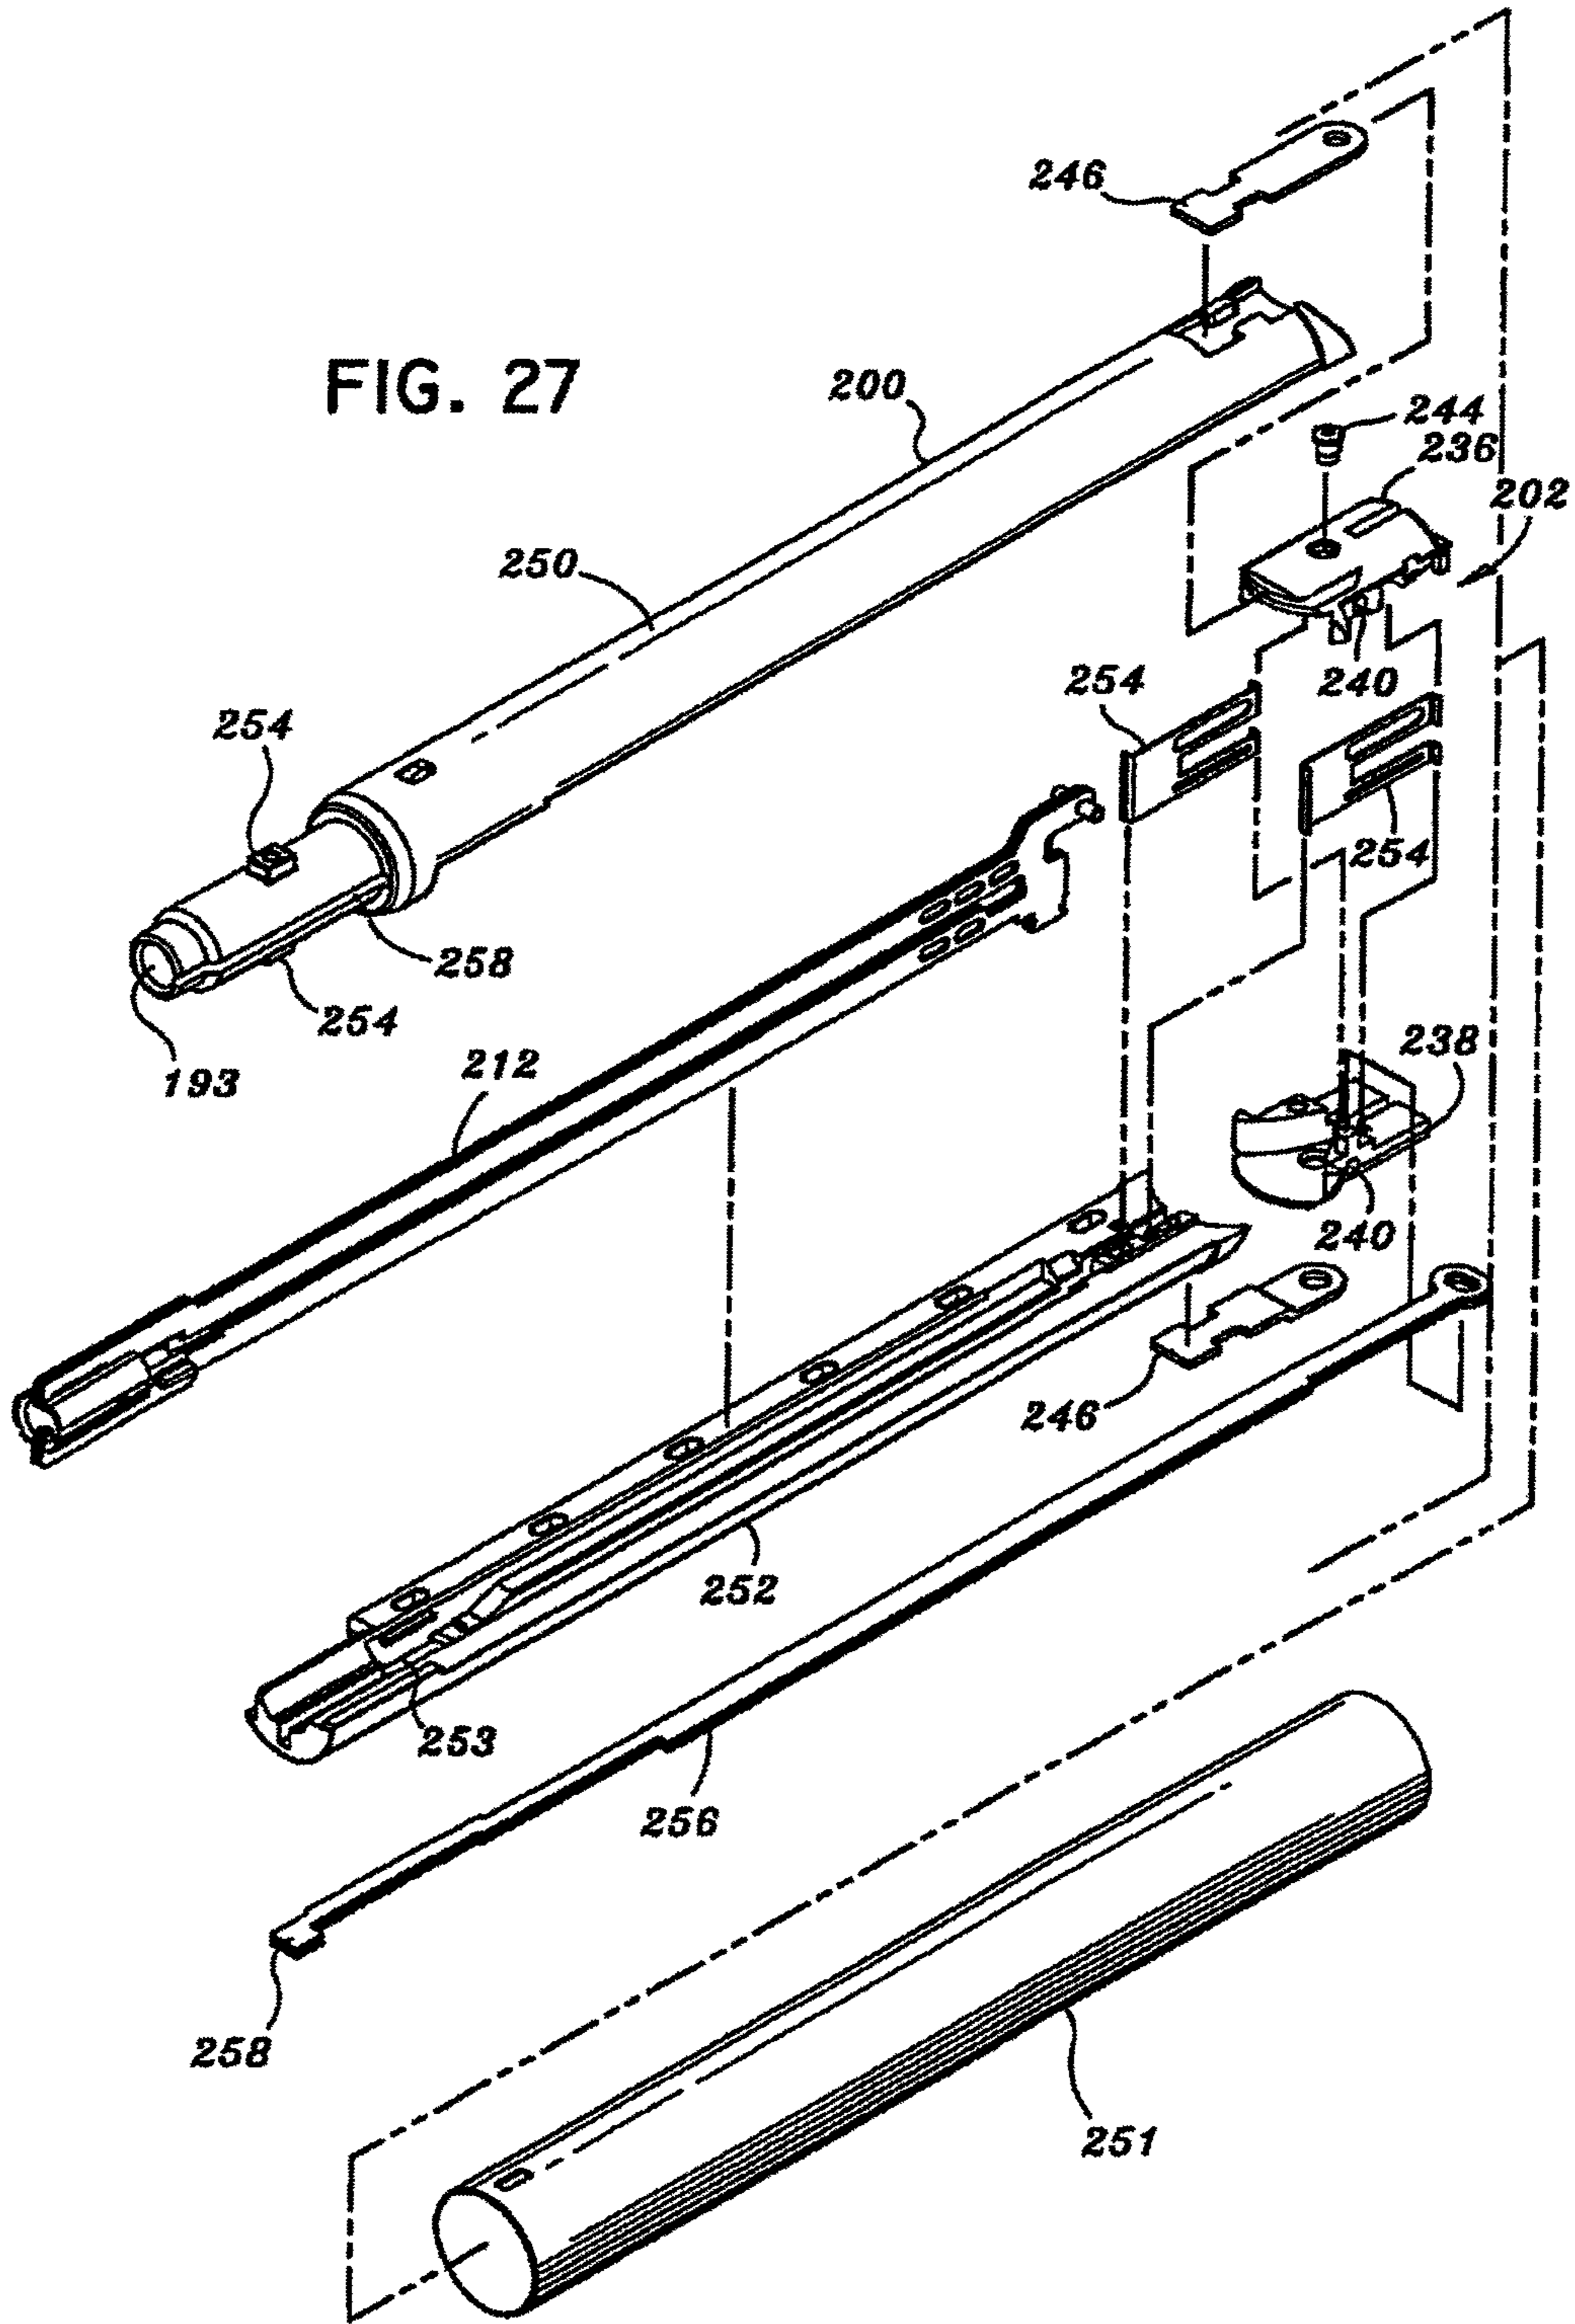
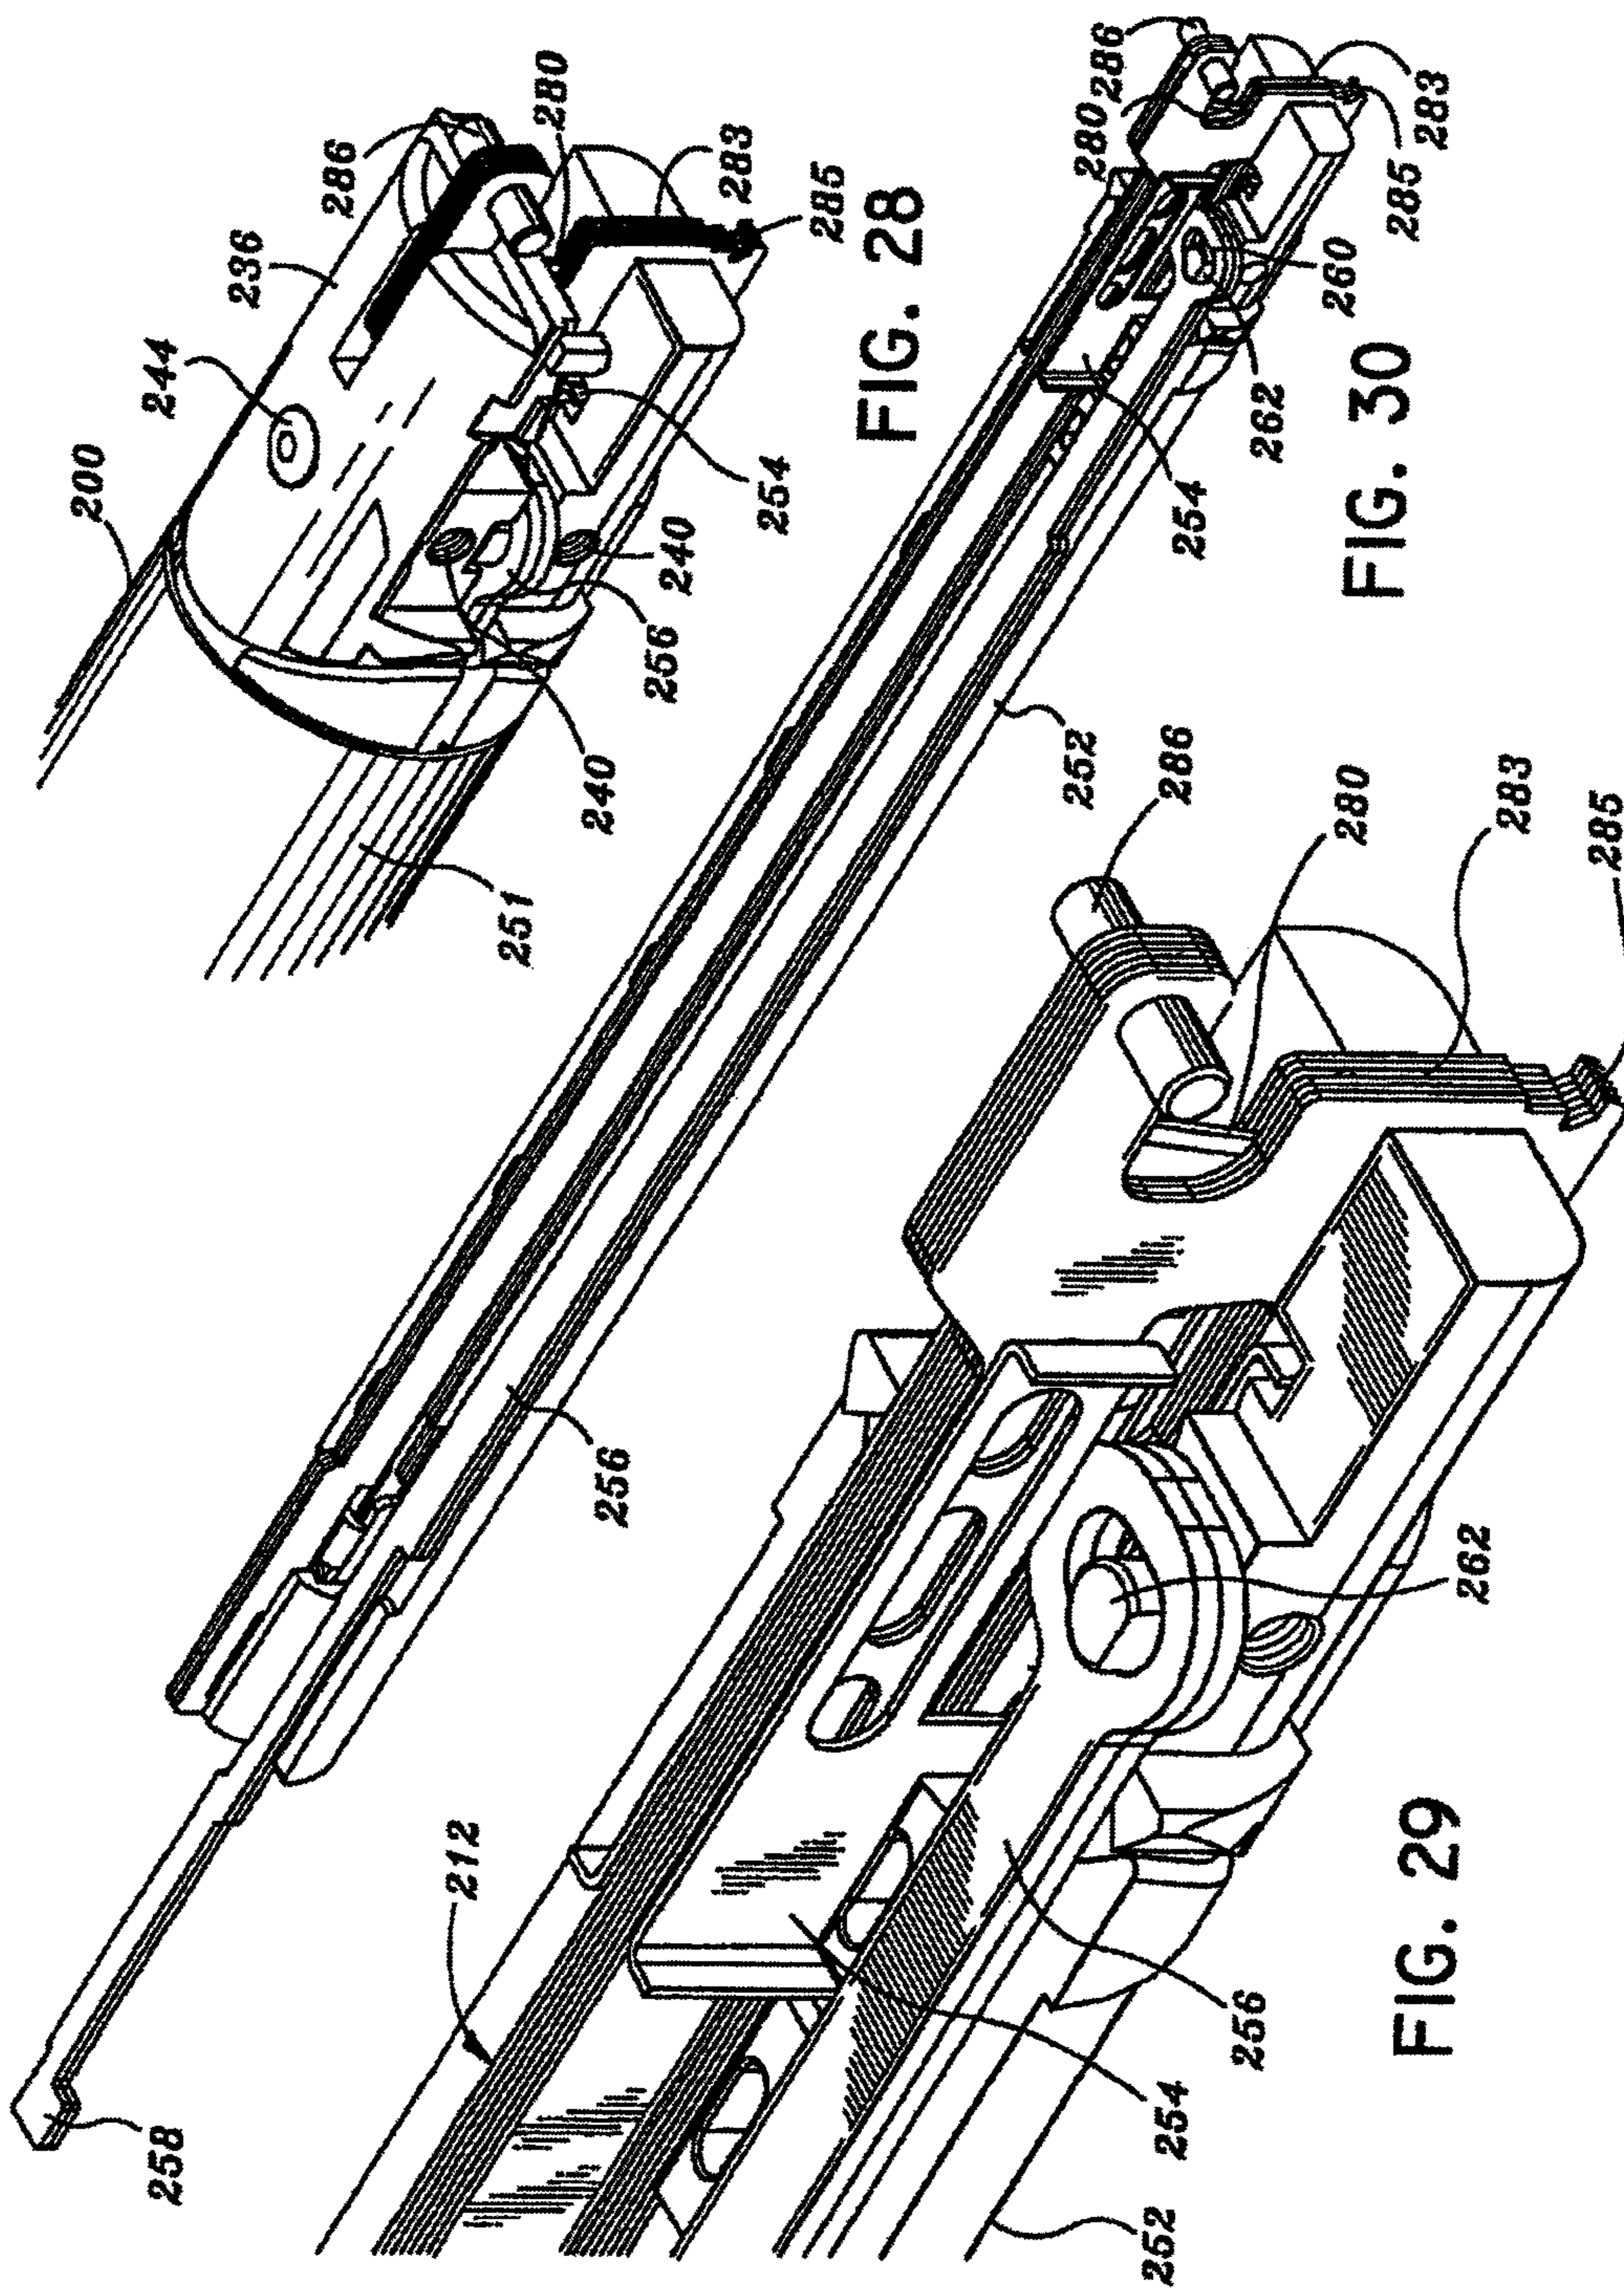


FIG. 26





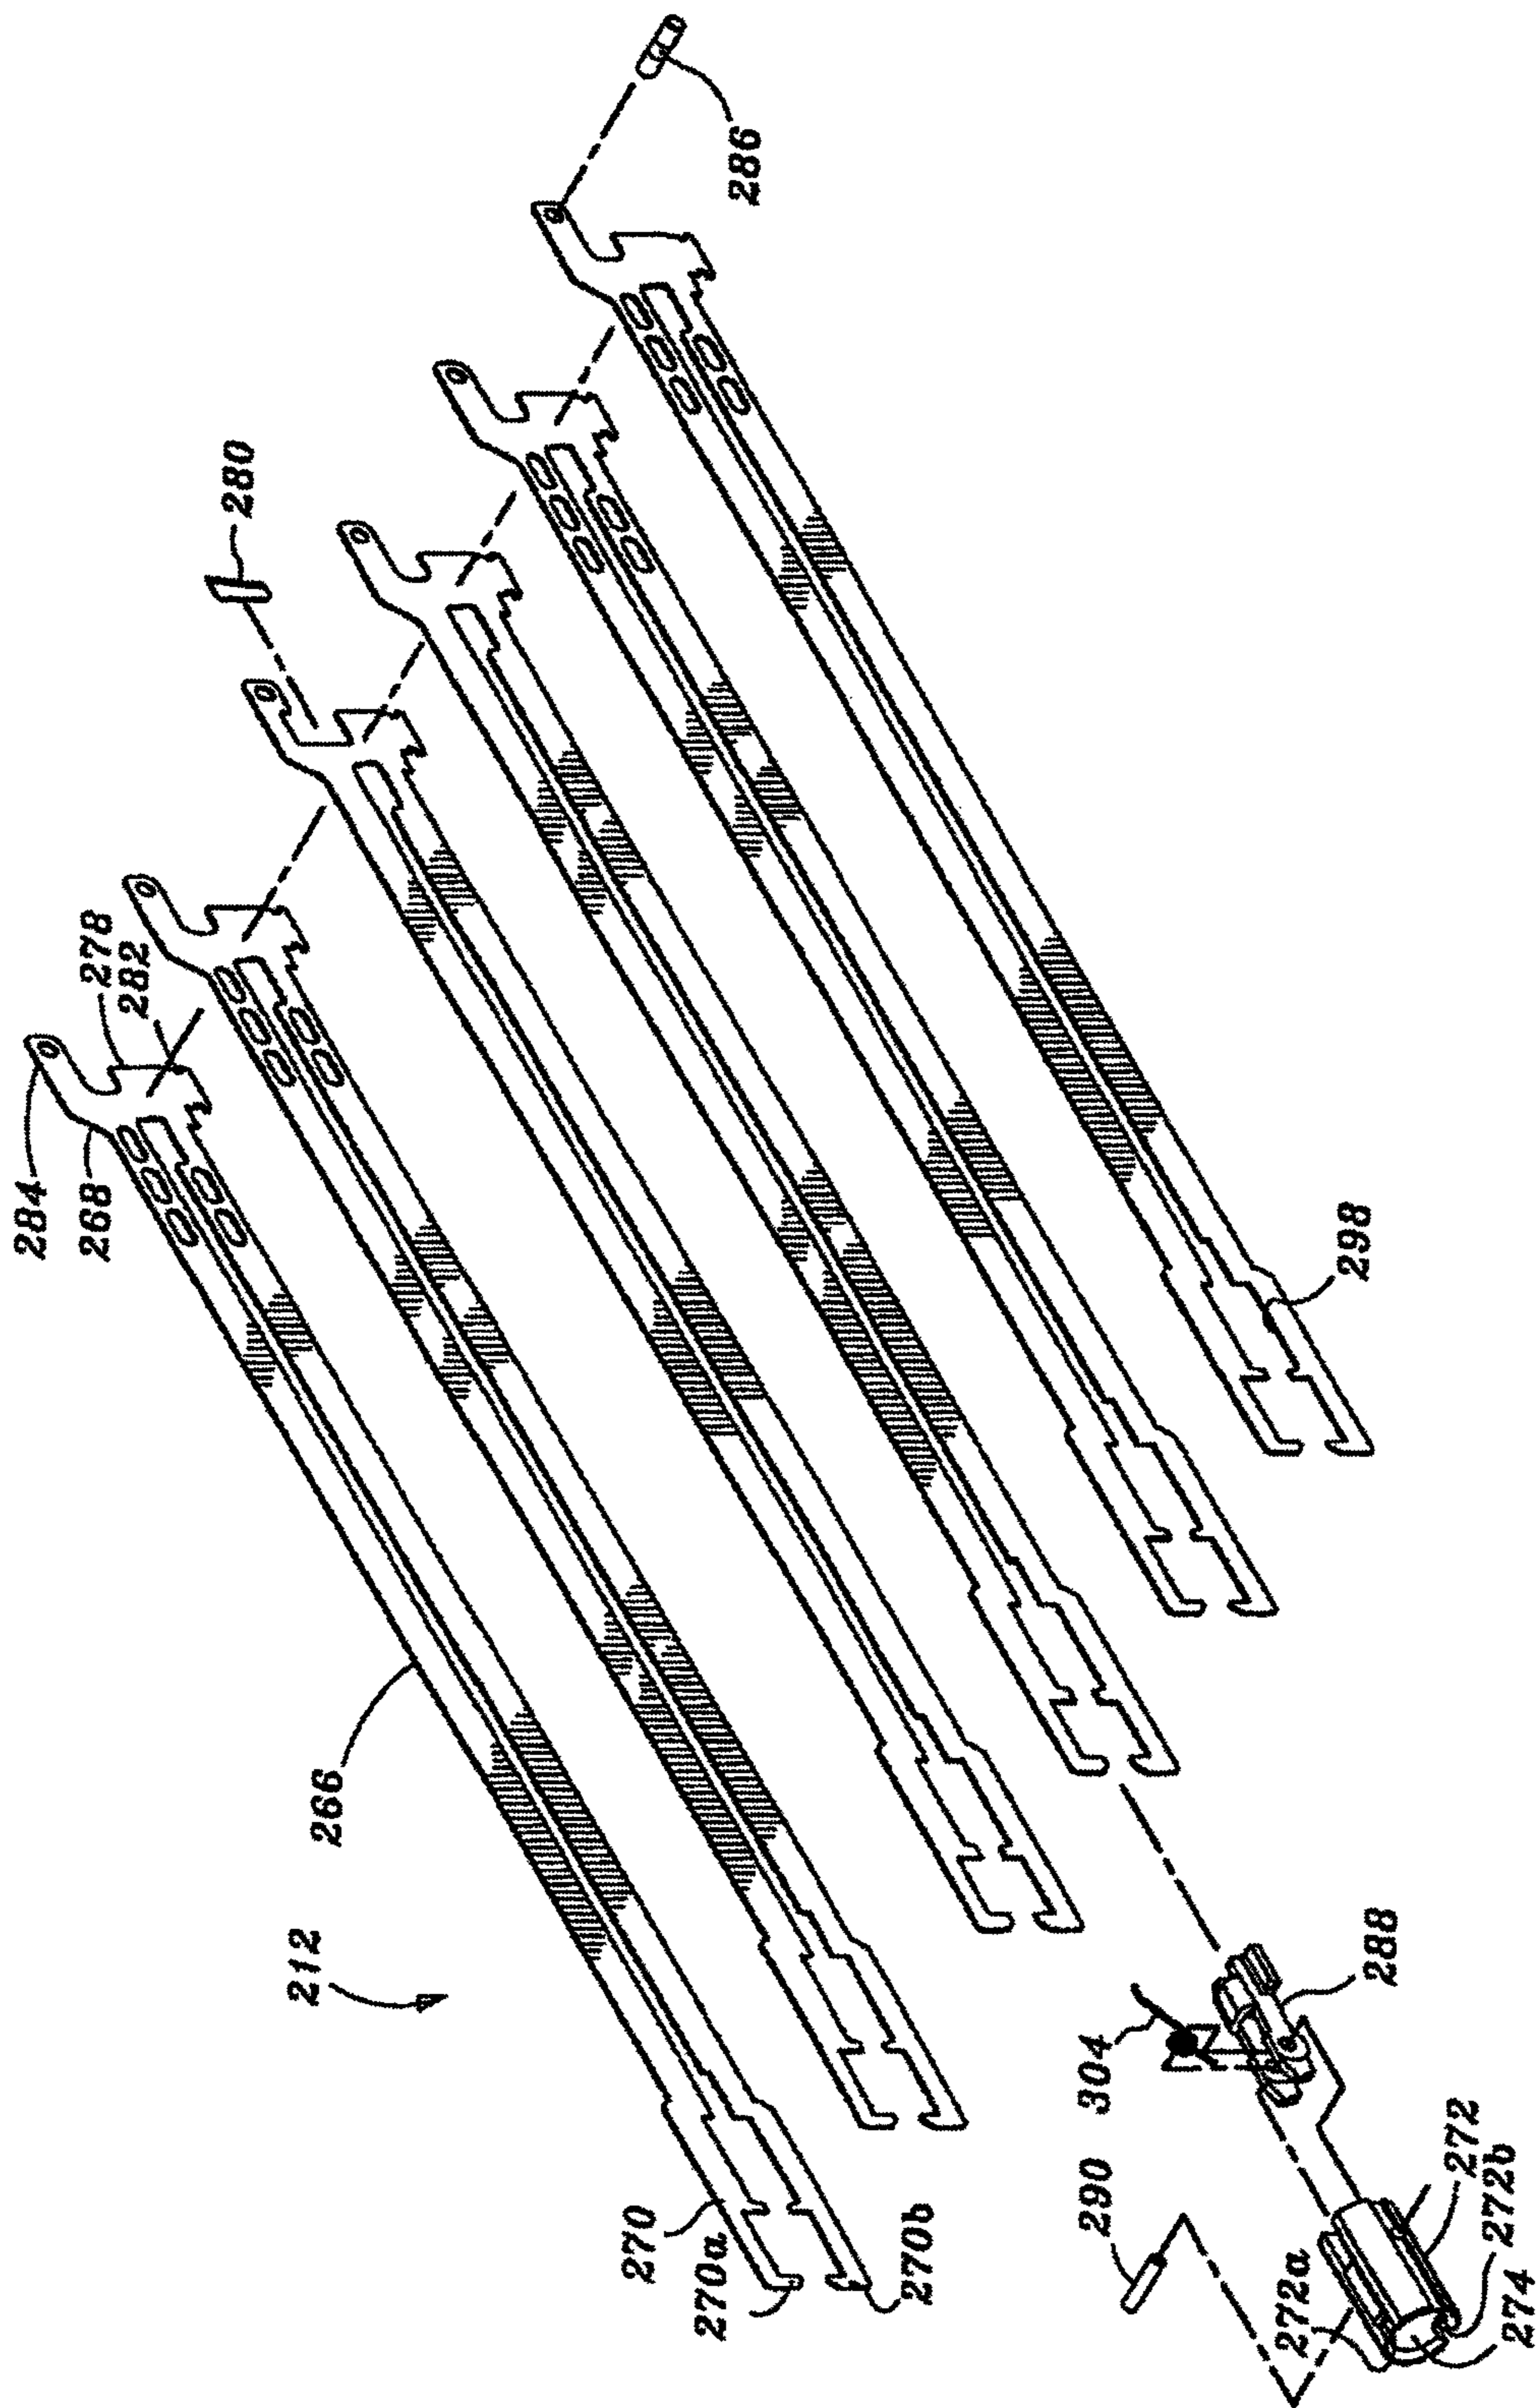


FIG. 31



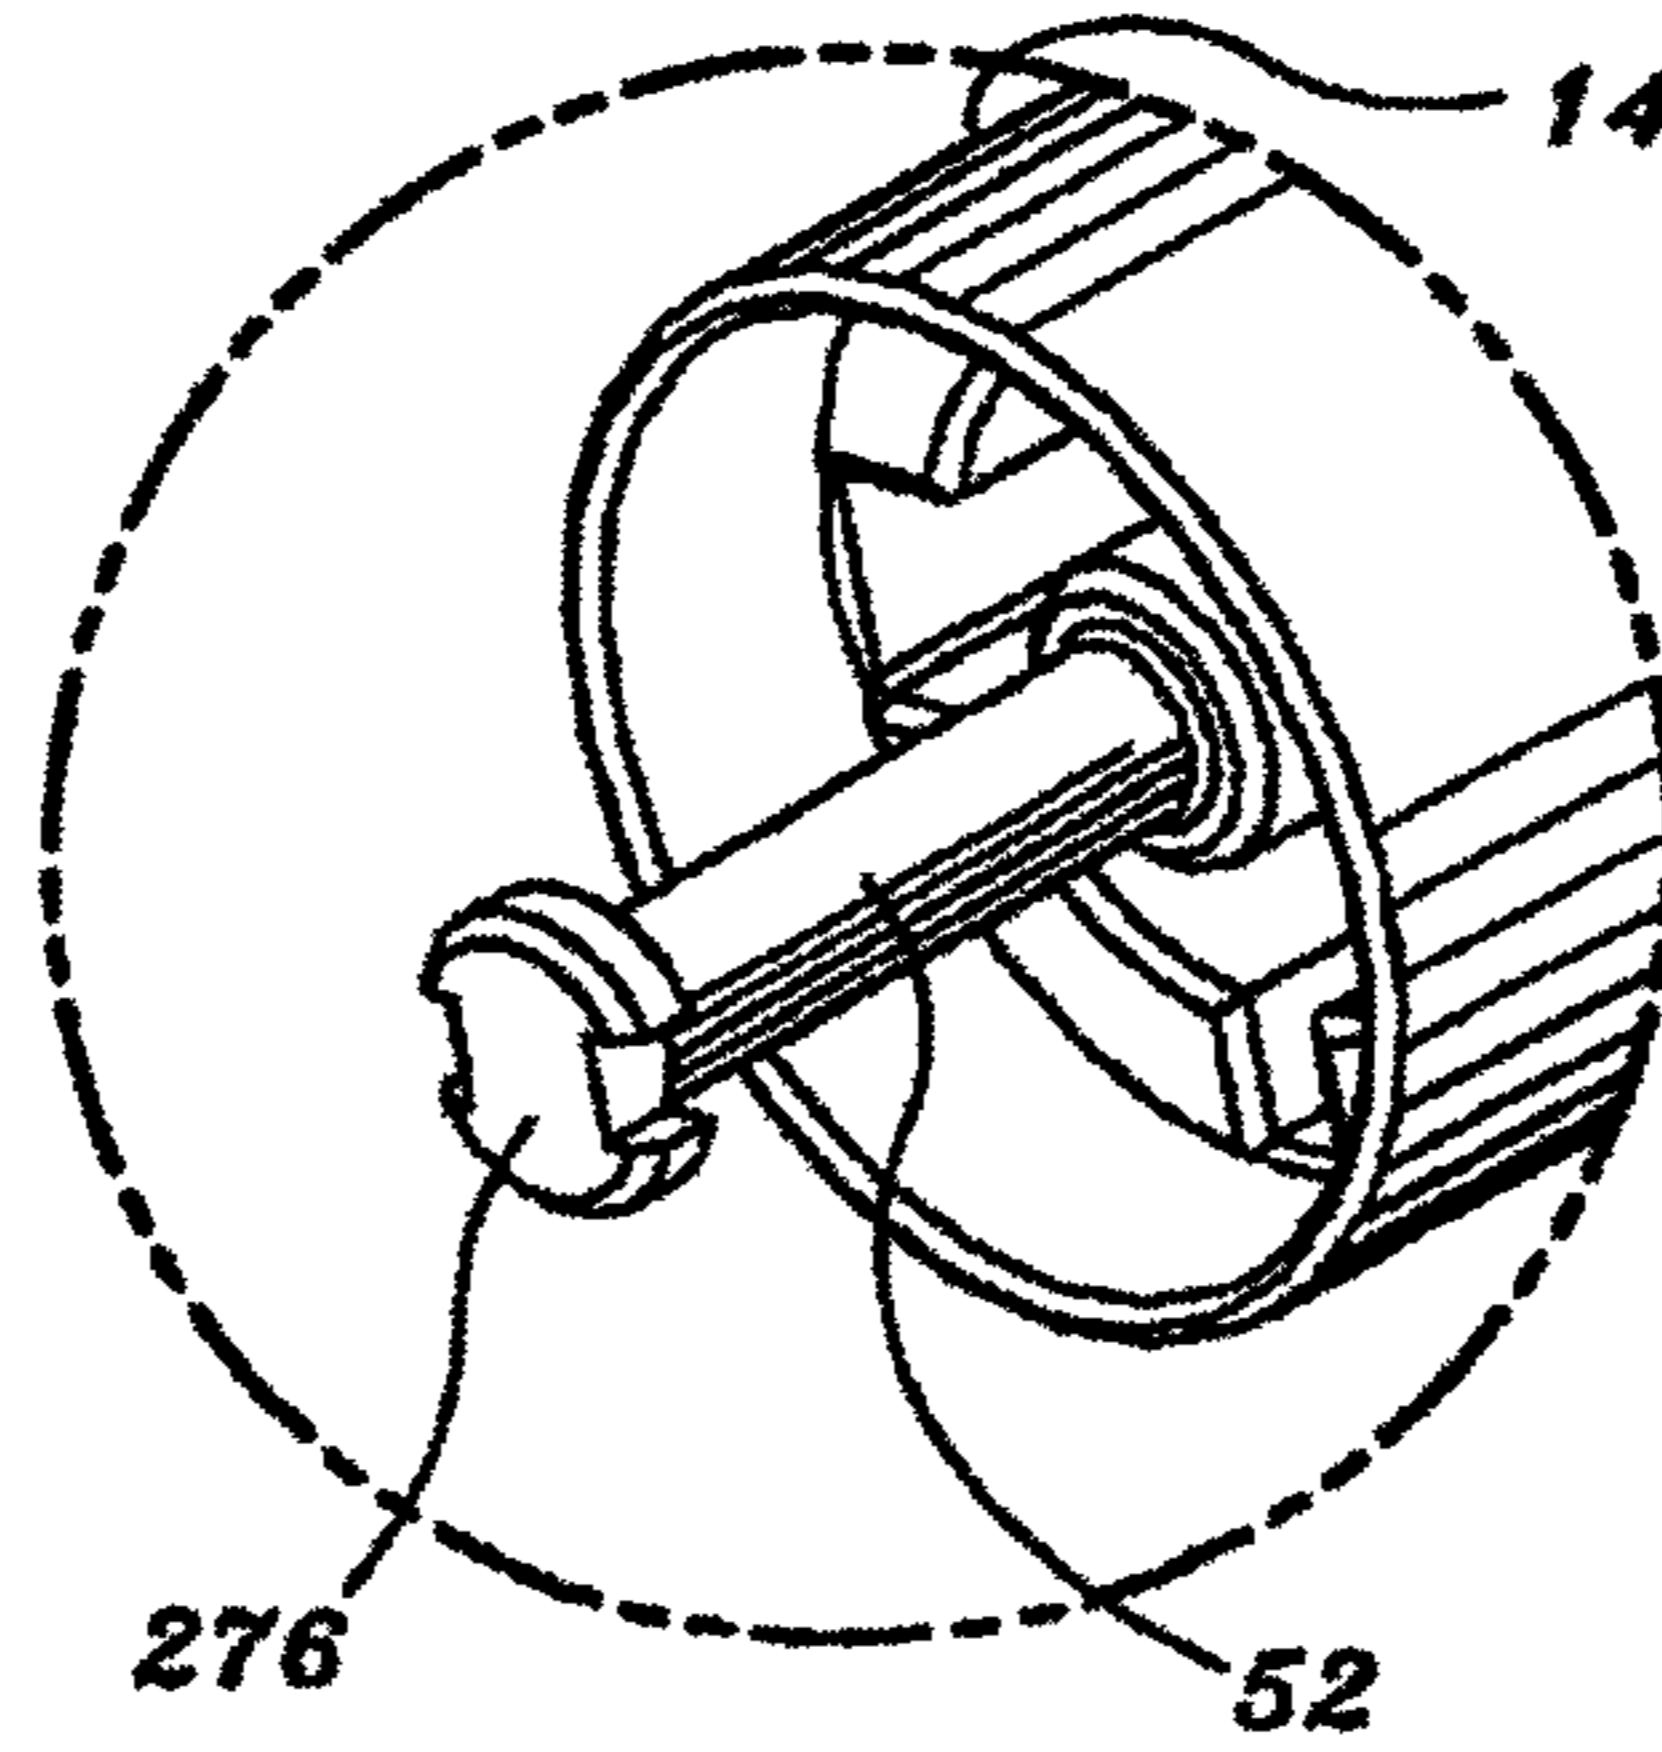


FIG. 35

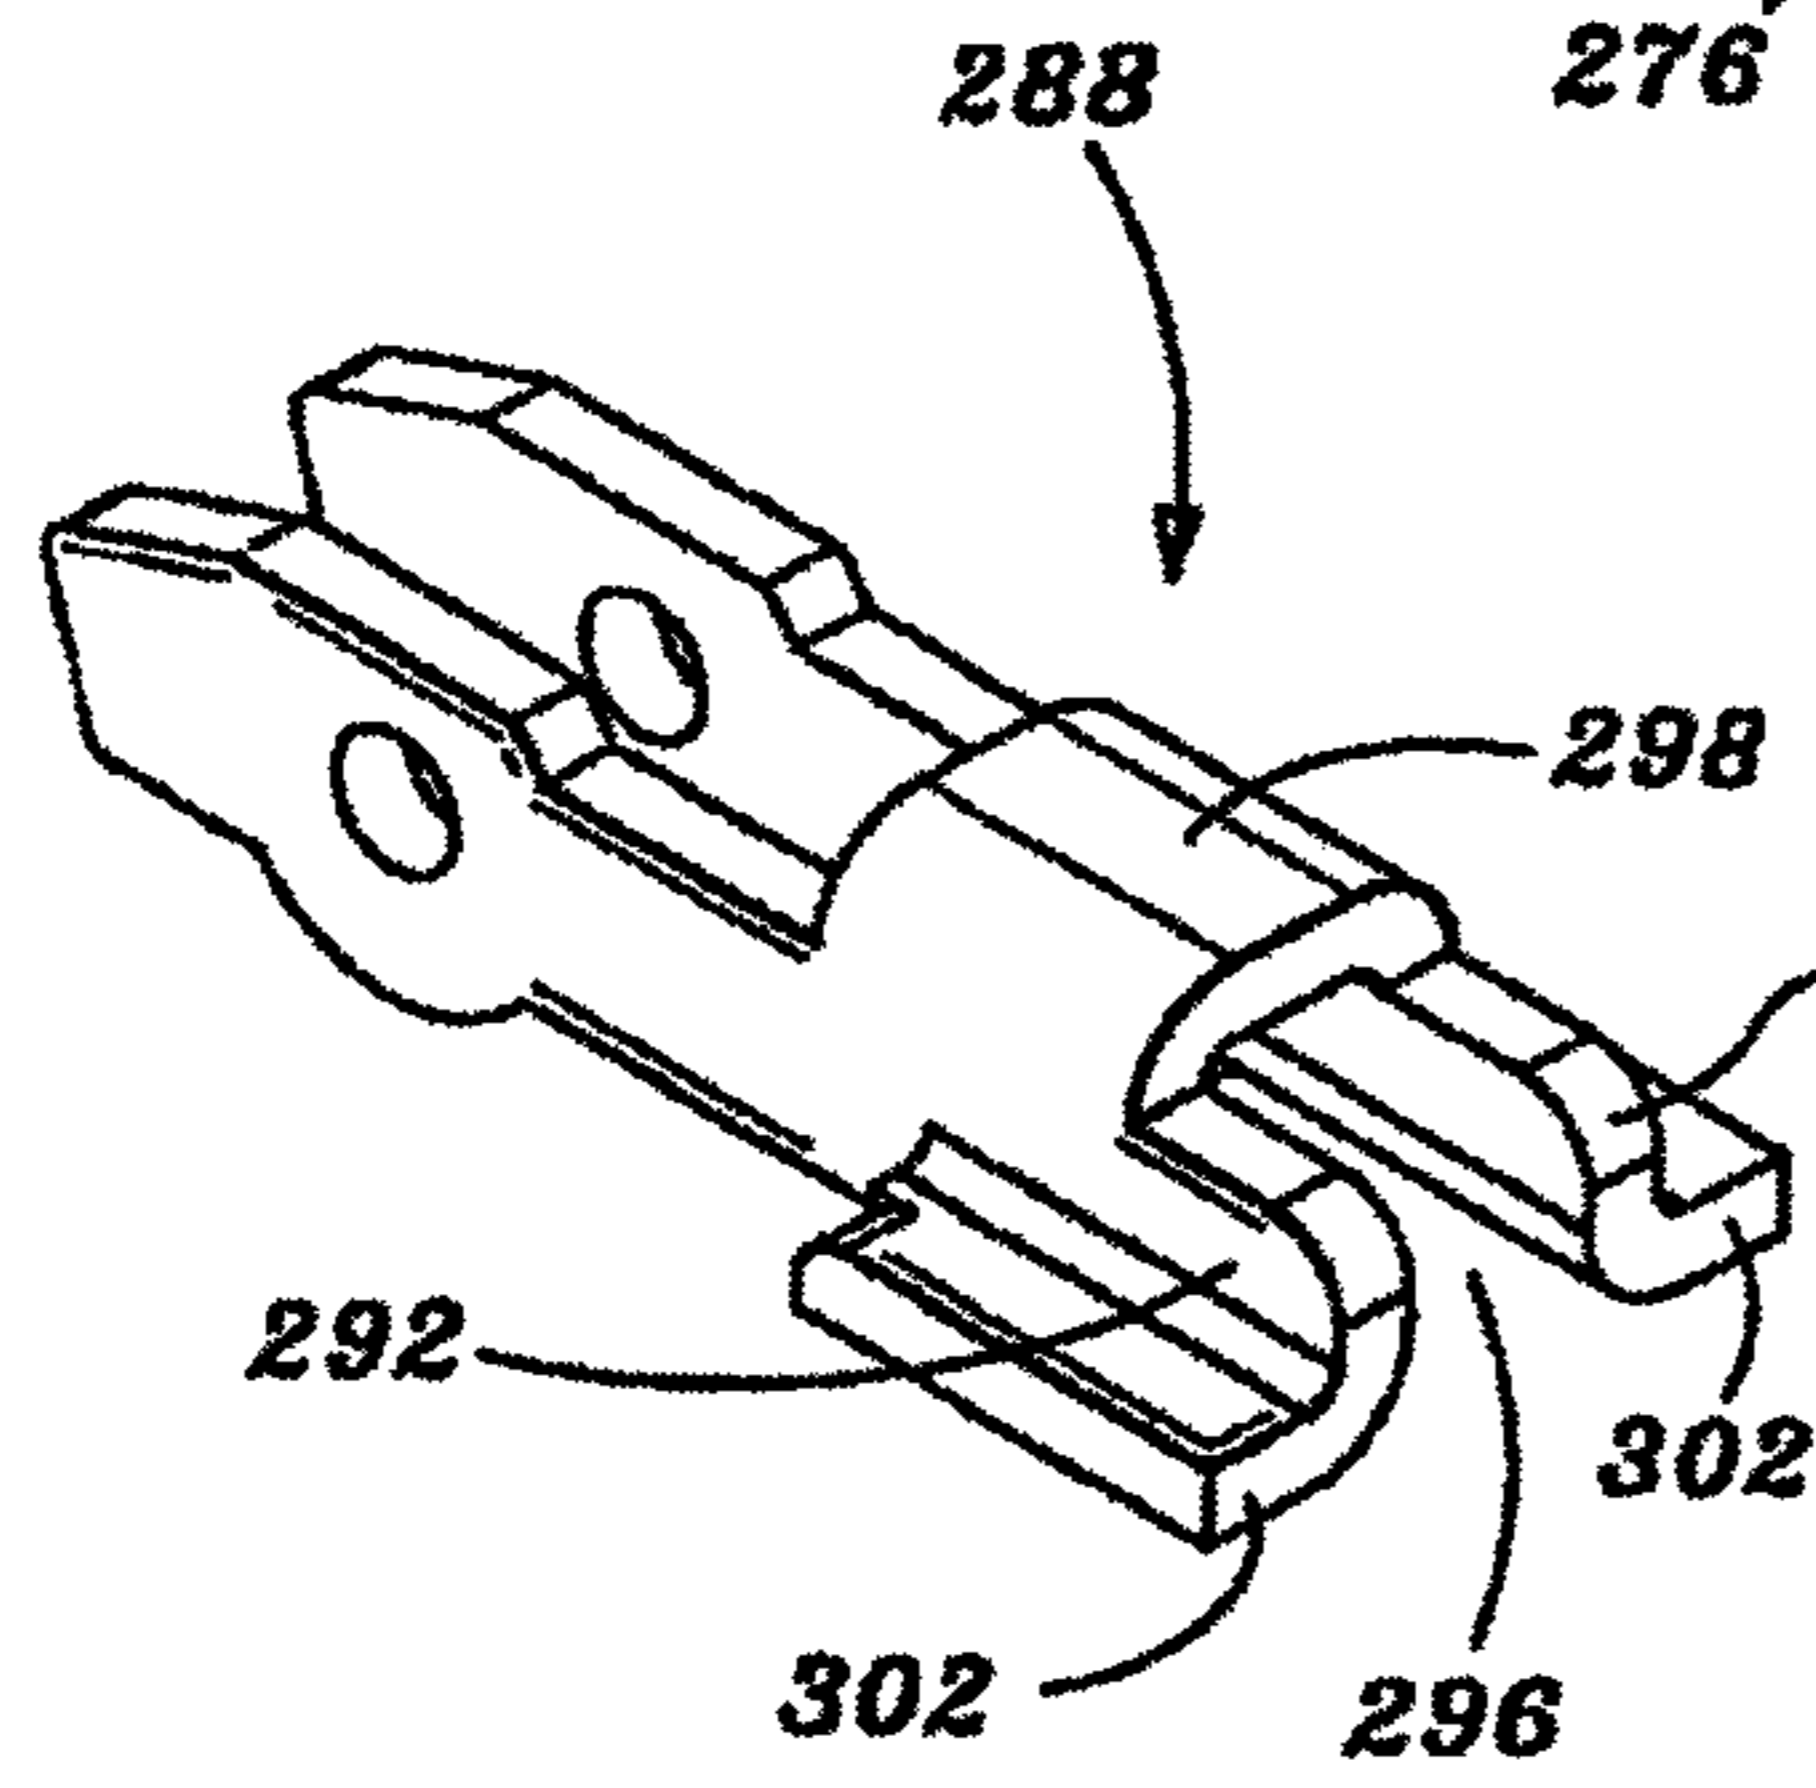


FIG. 36

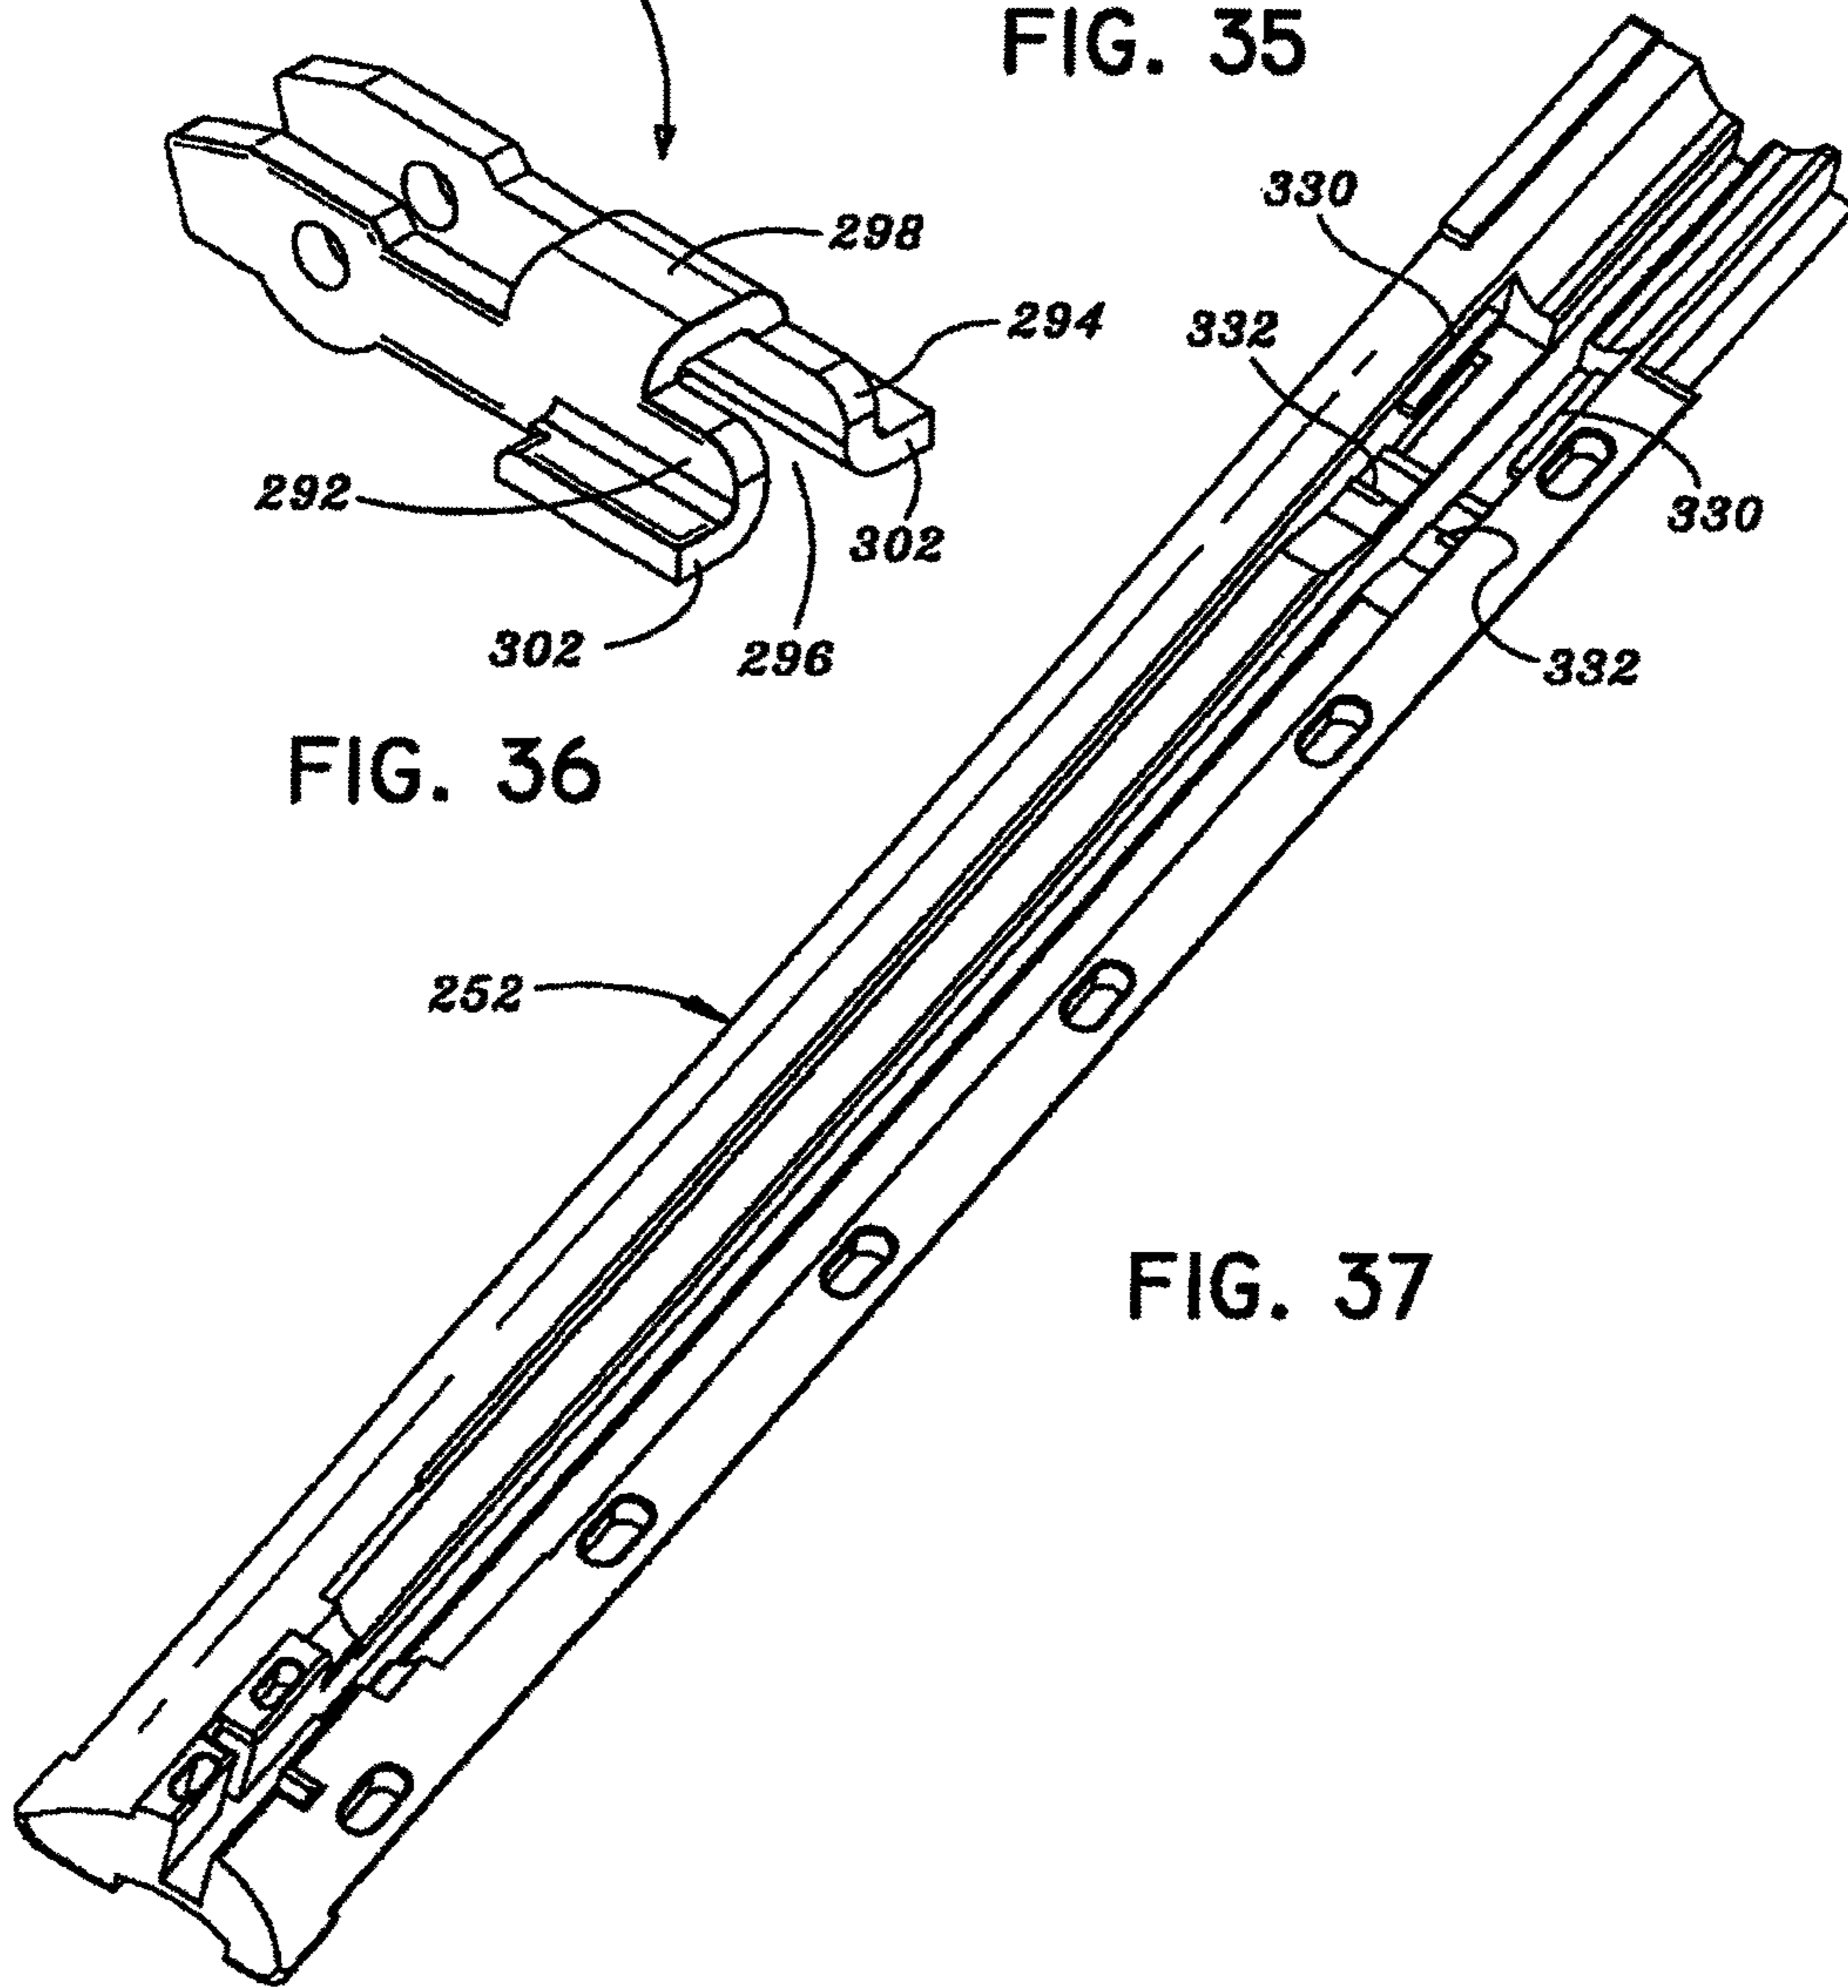


FIG. 37

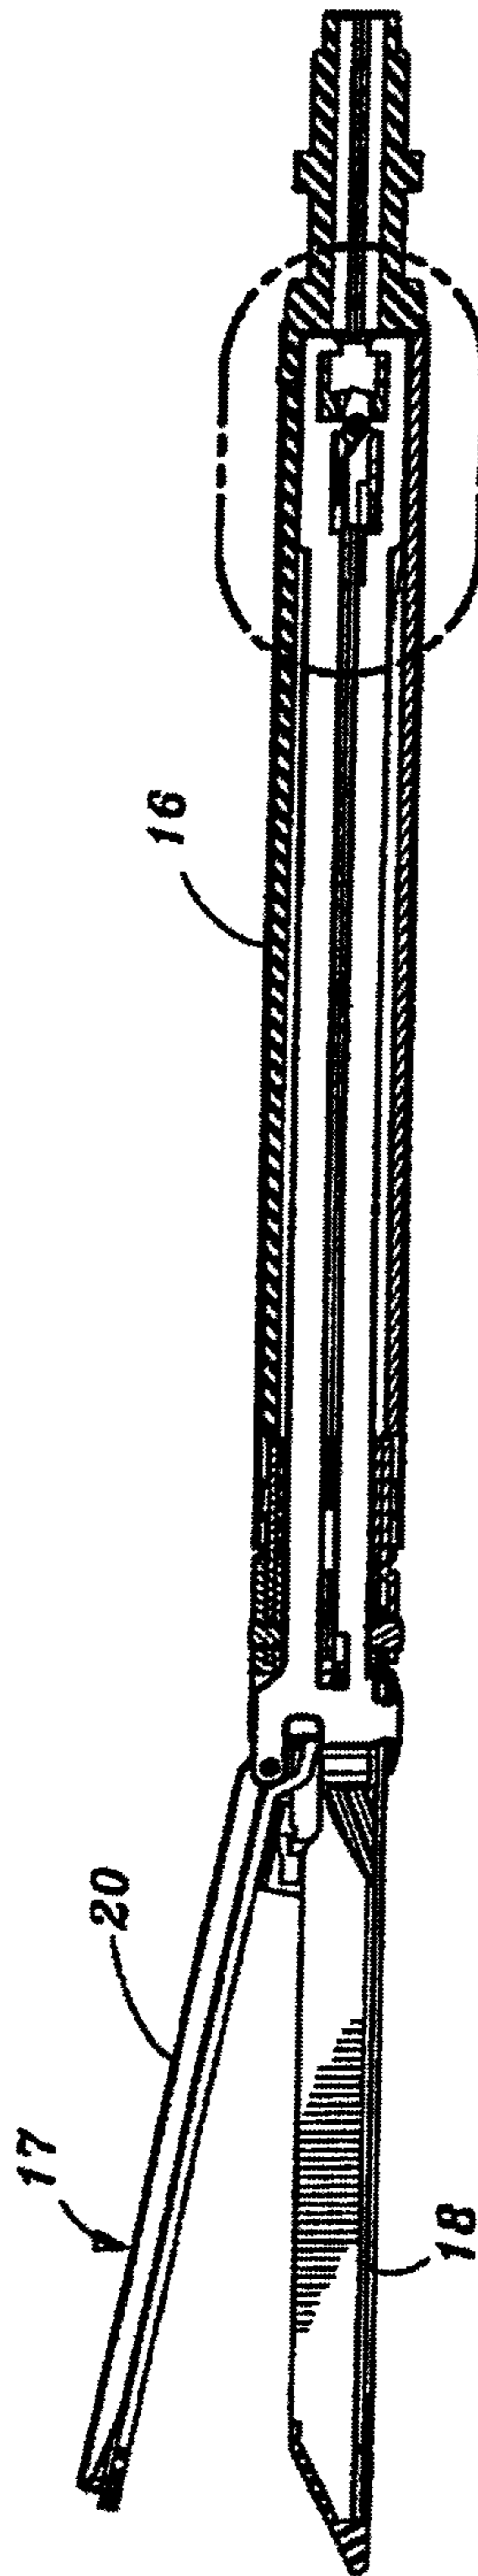


FIG. 38

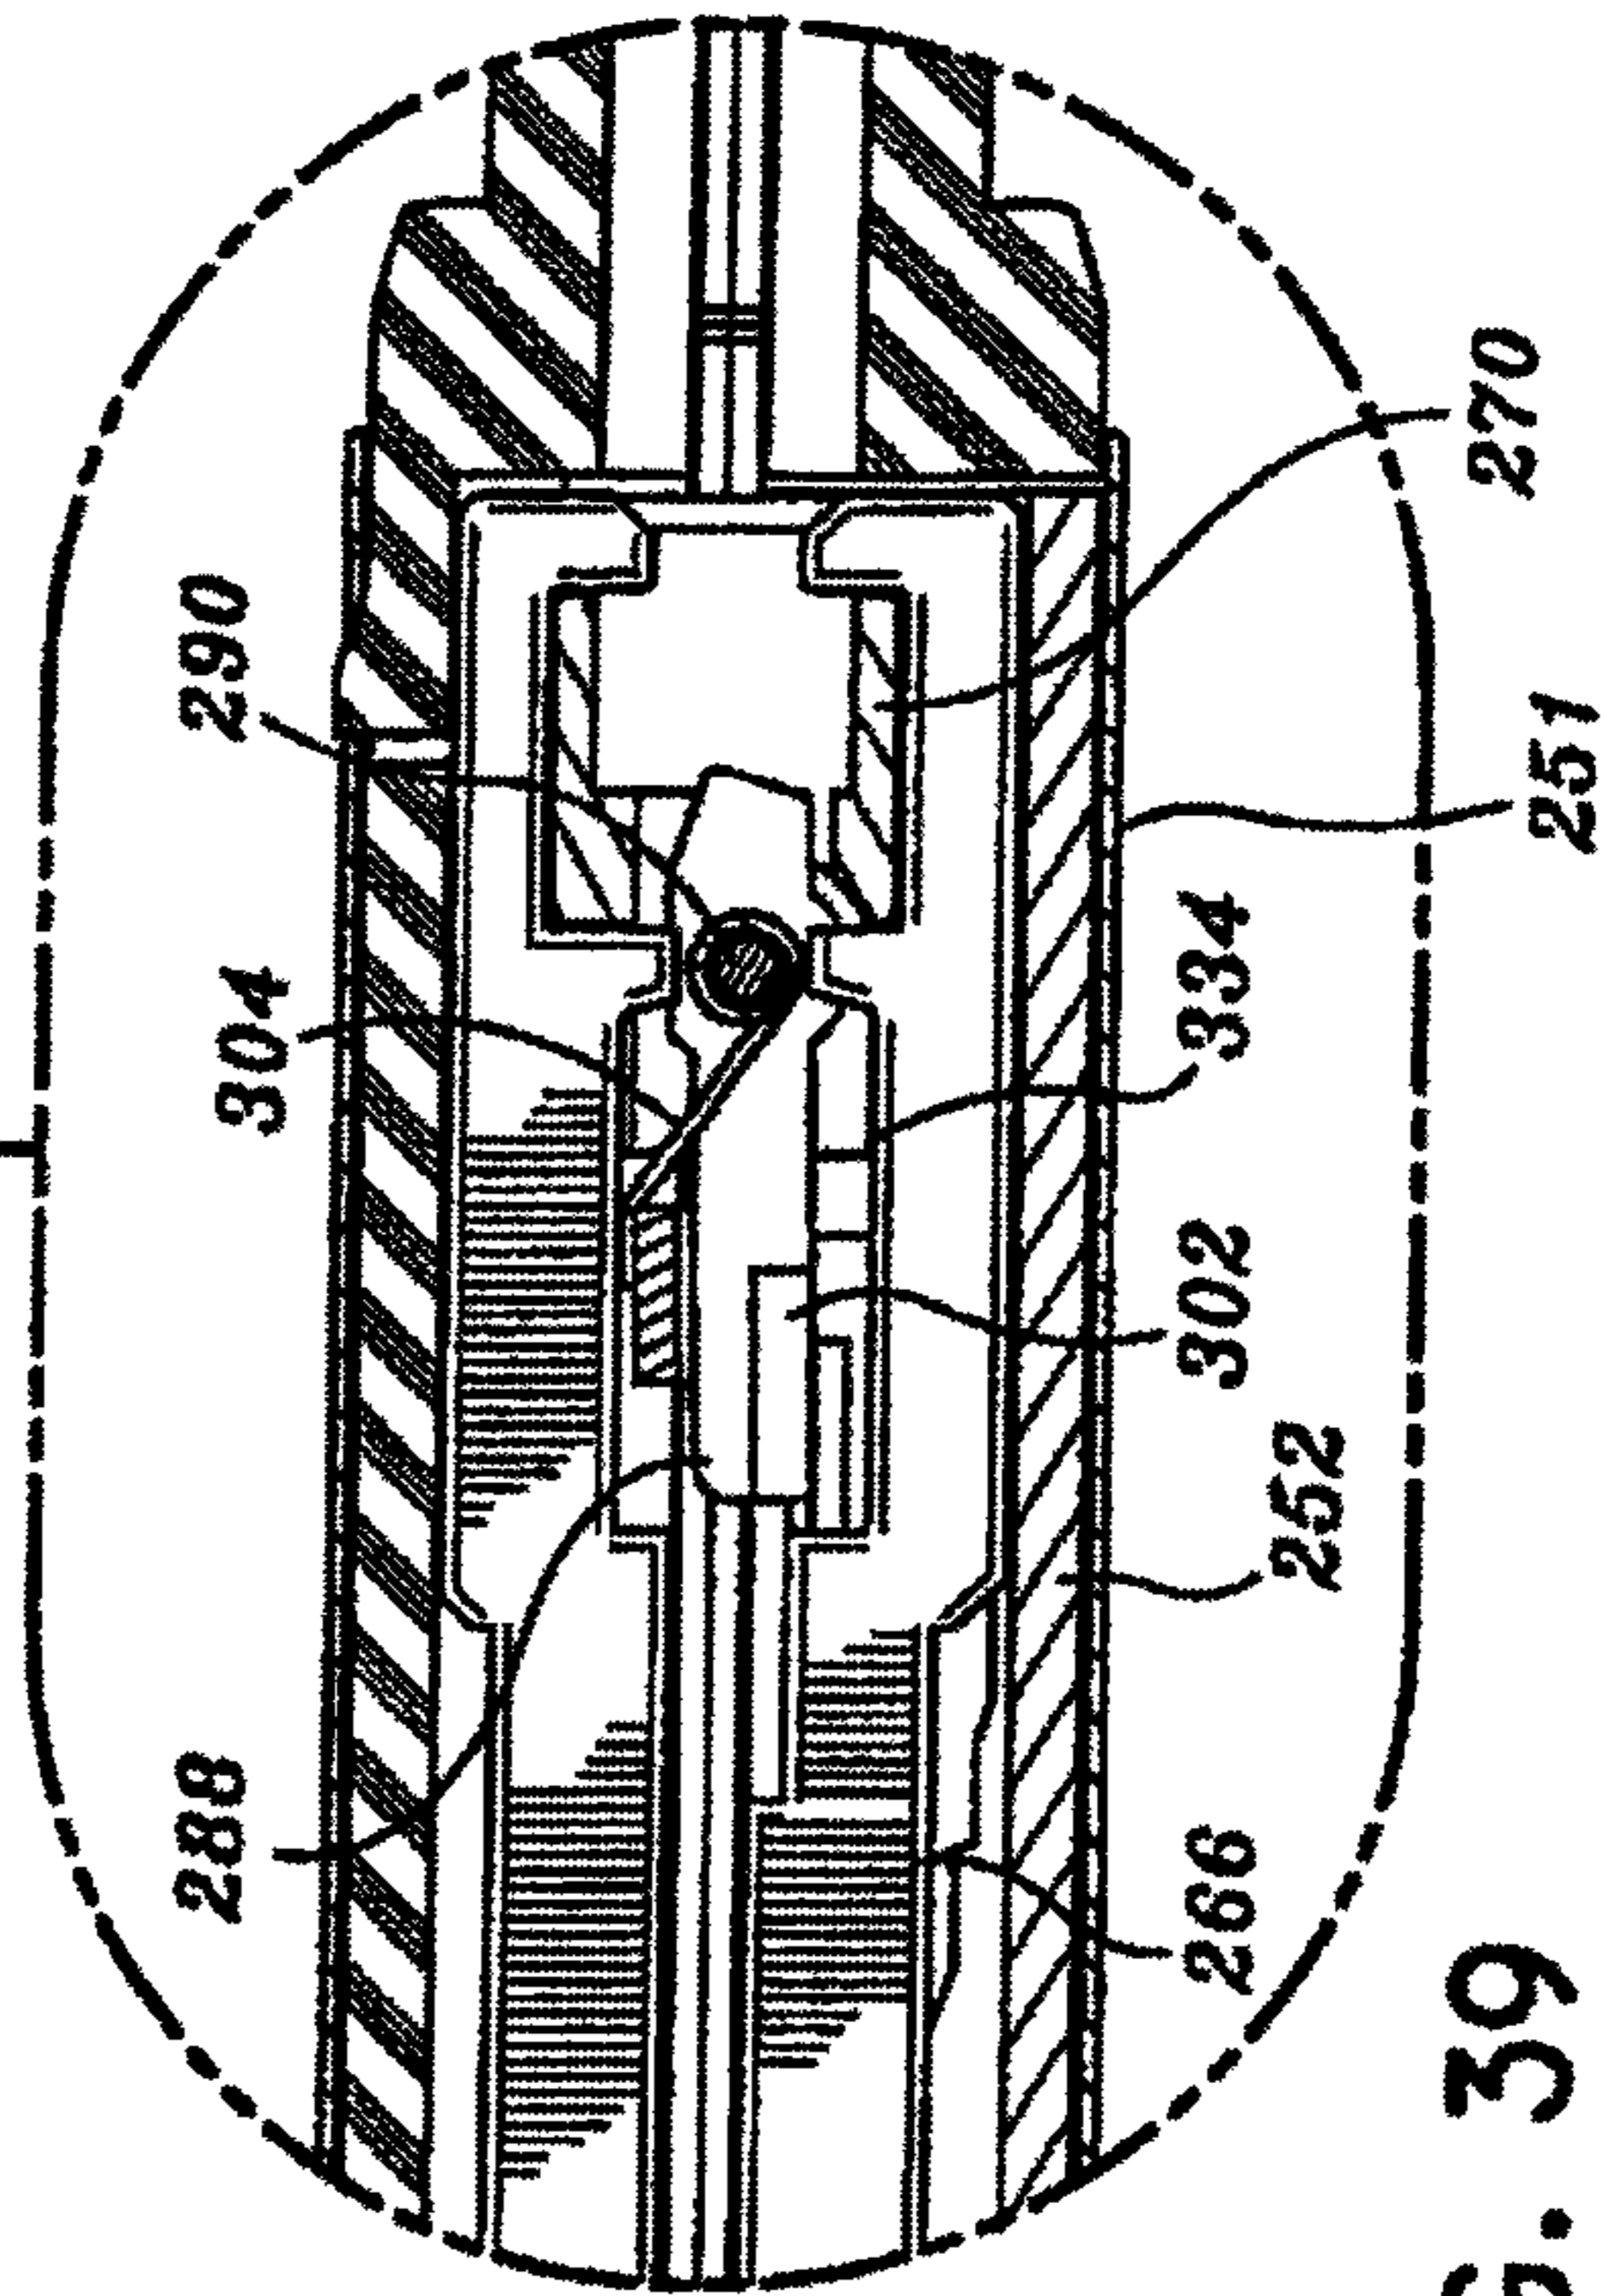


FIG. 39



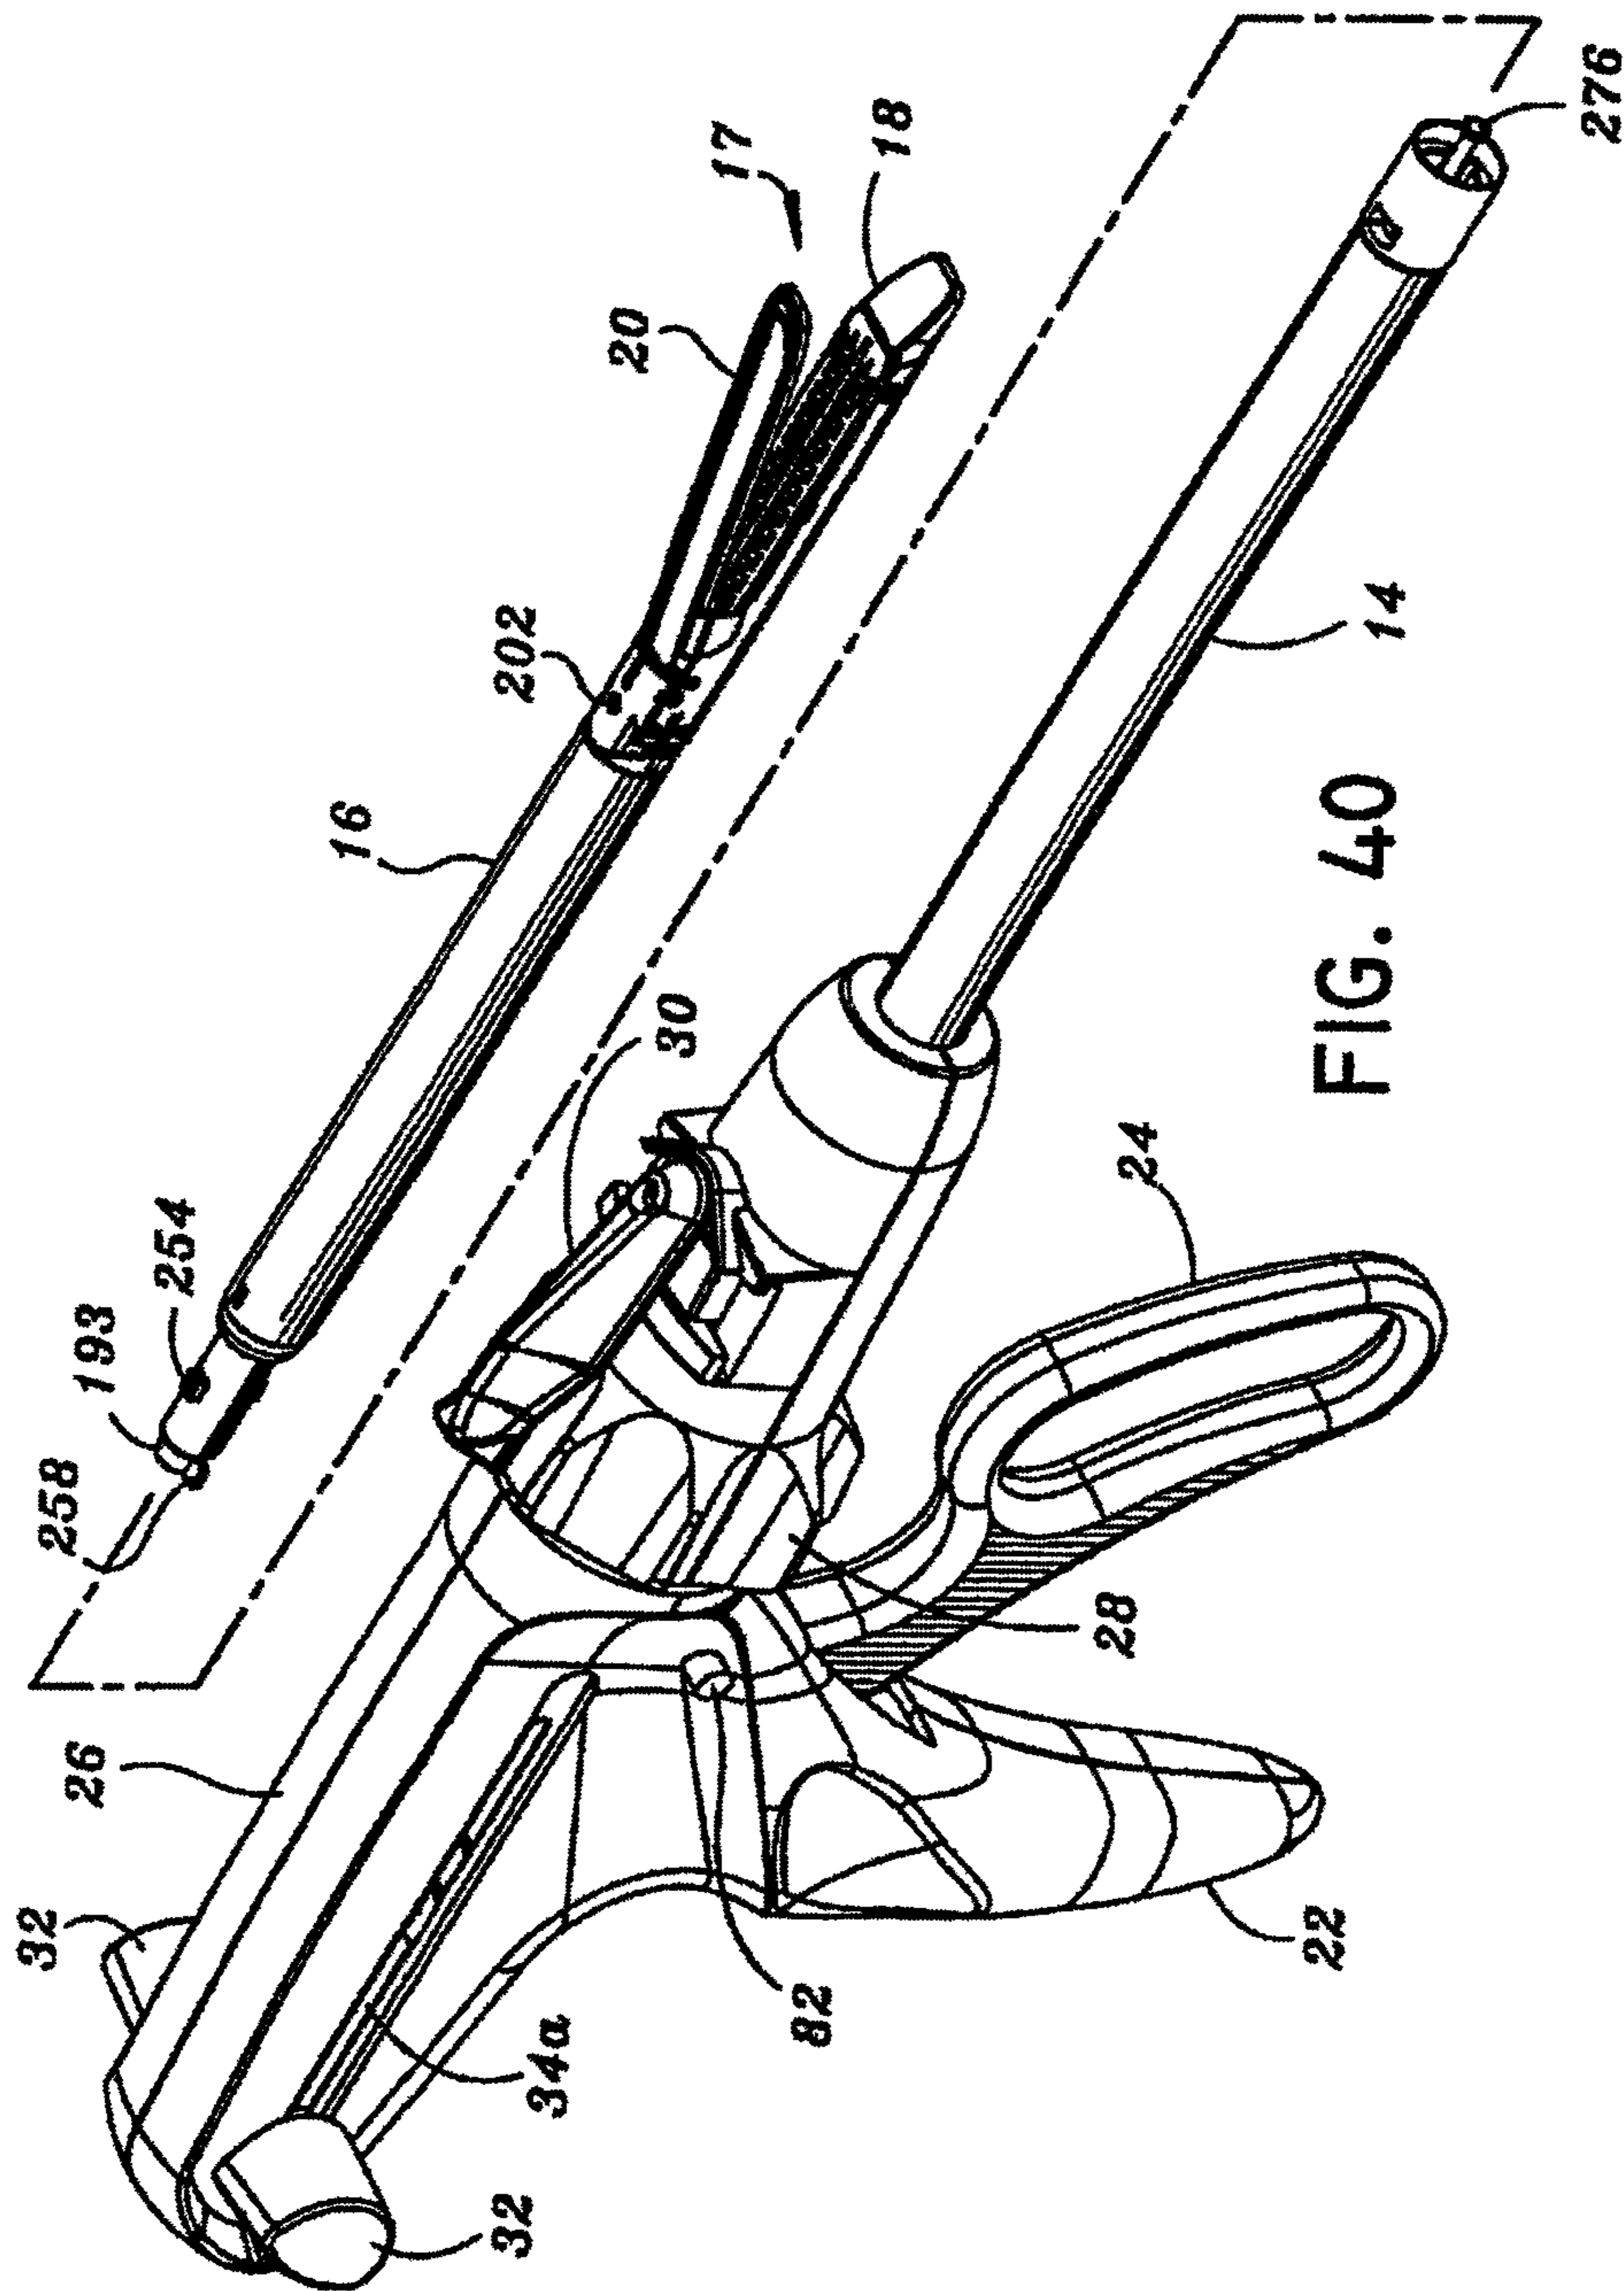
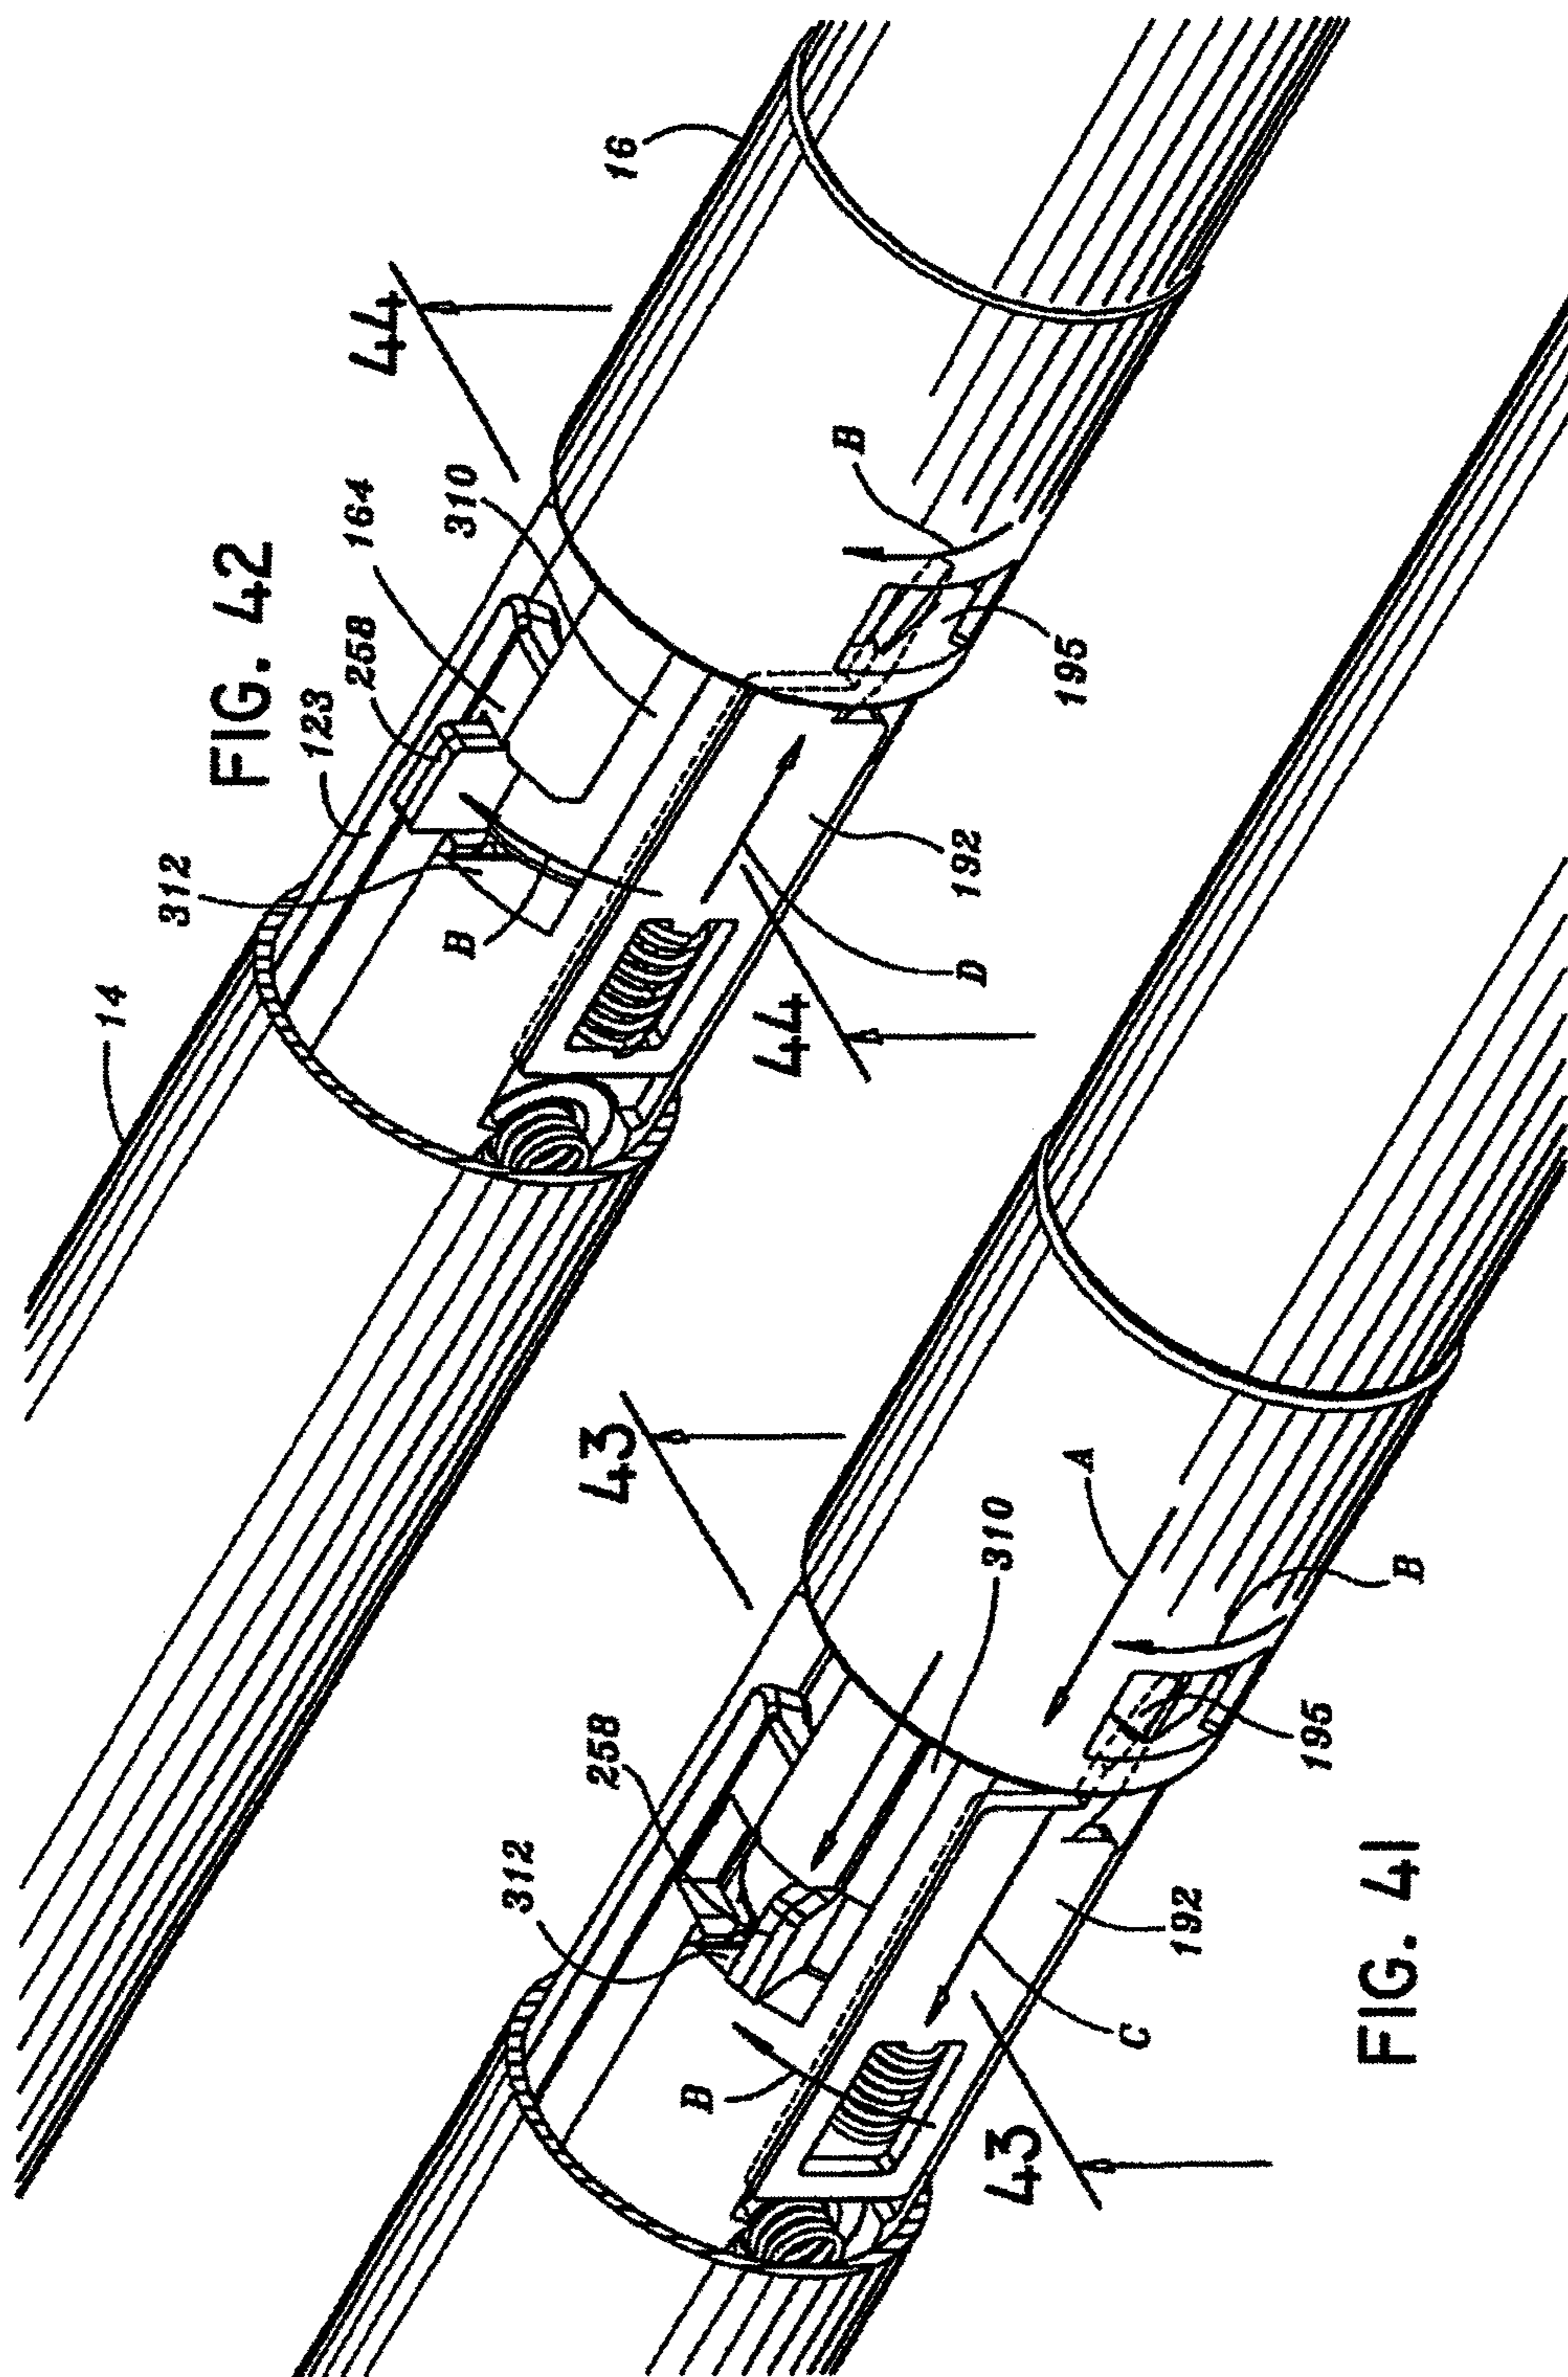


FIG. 40



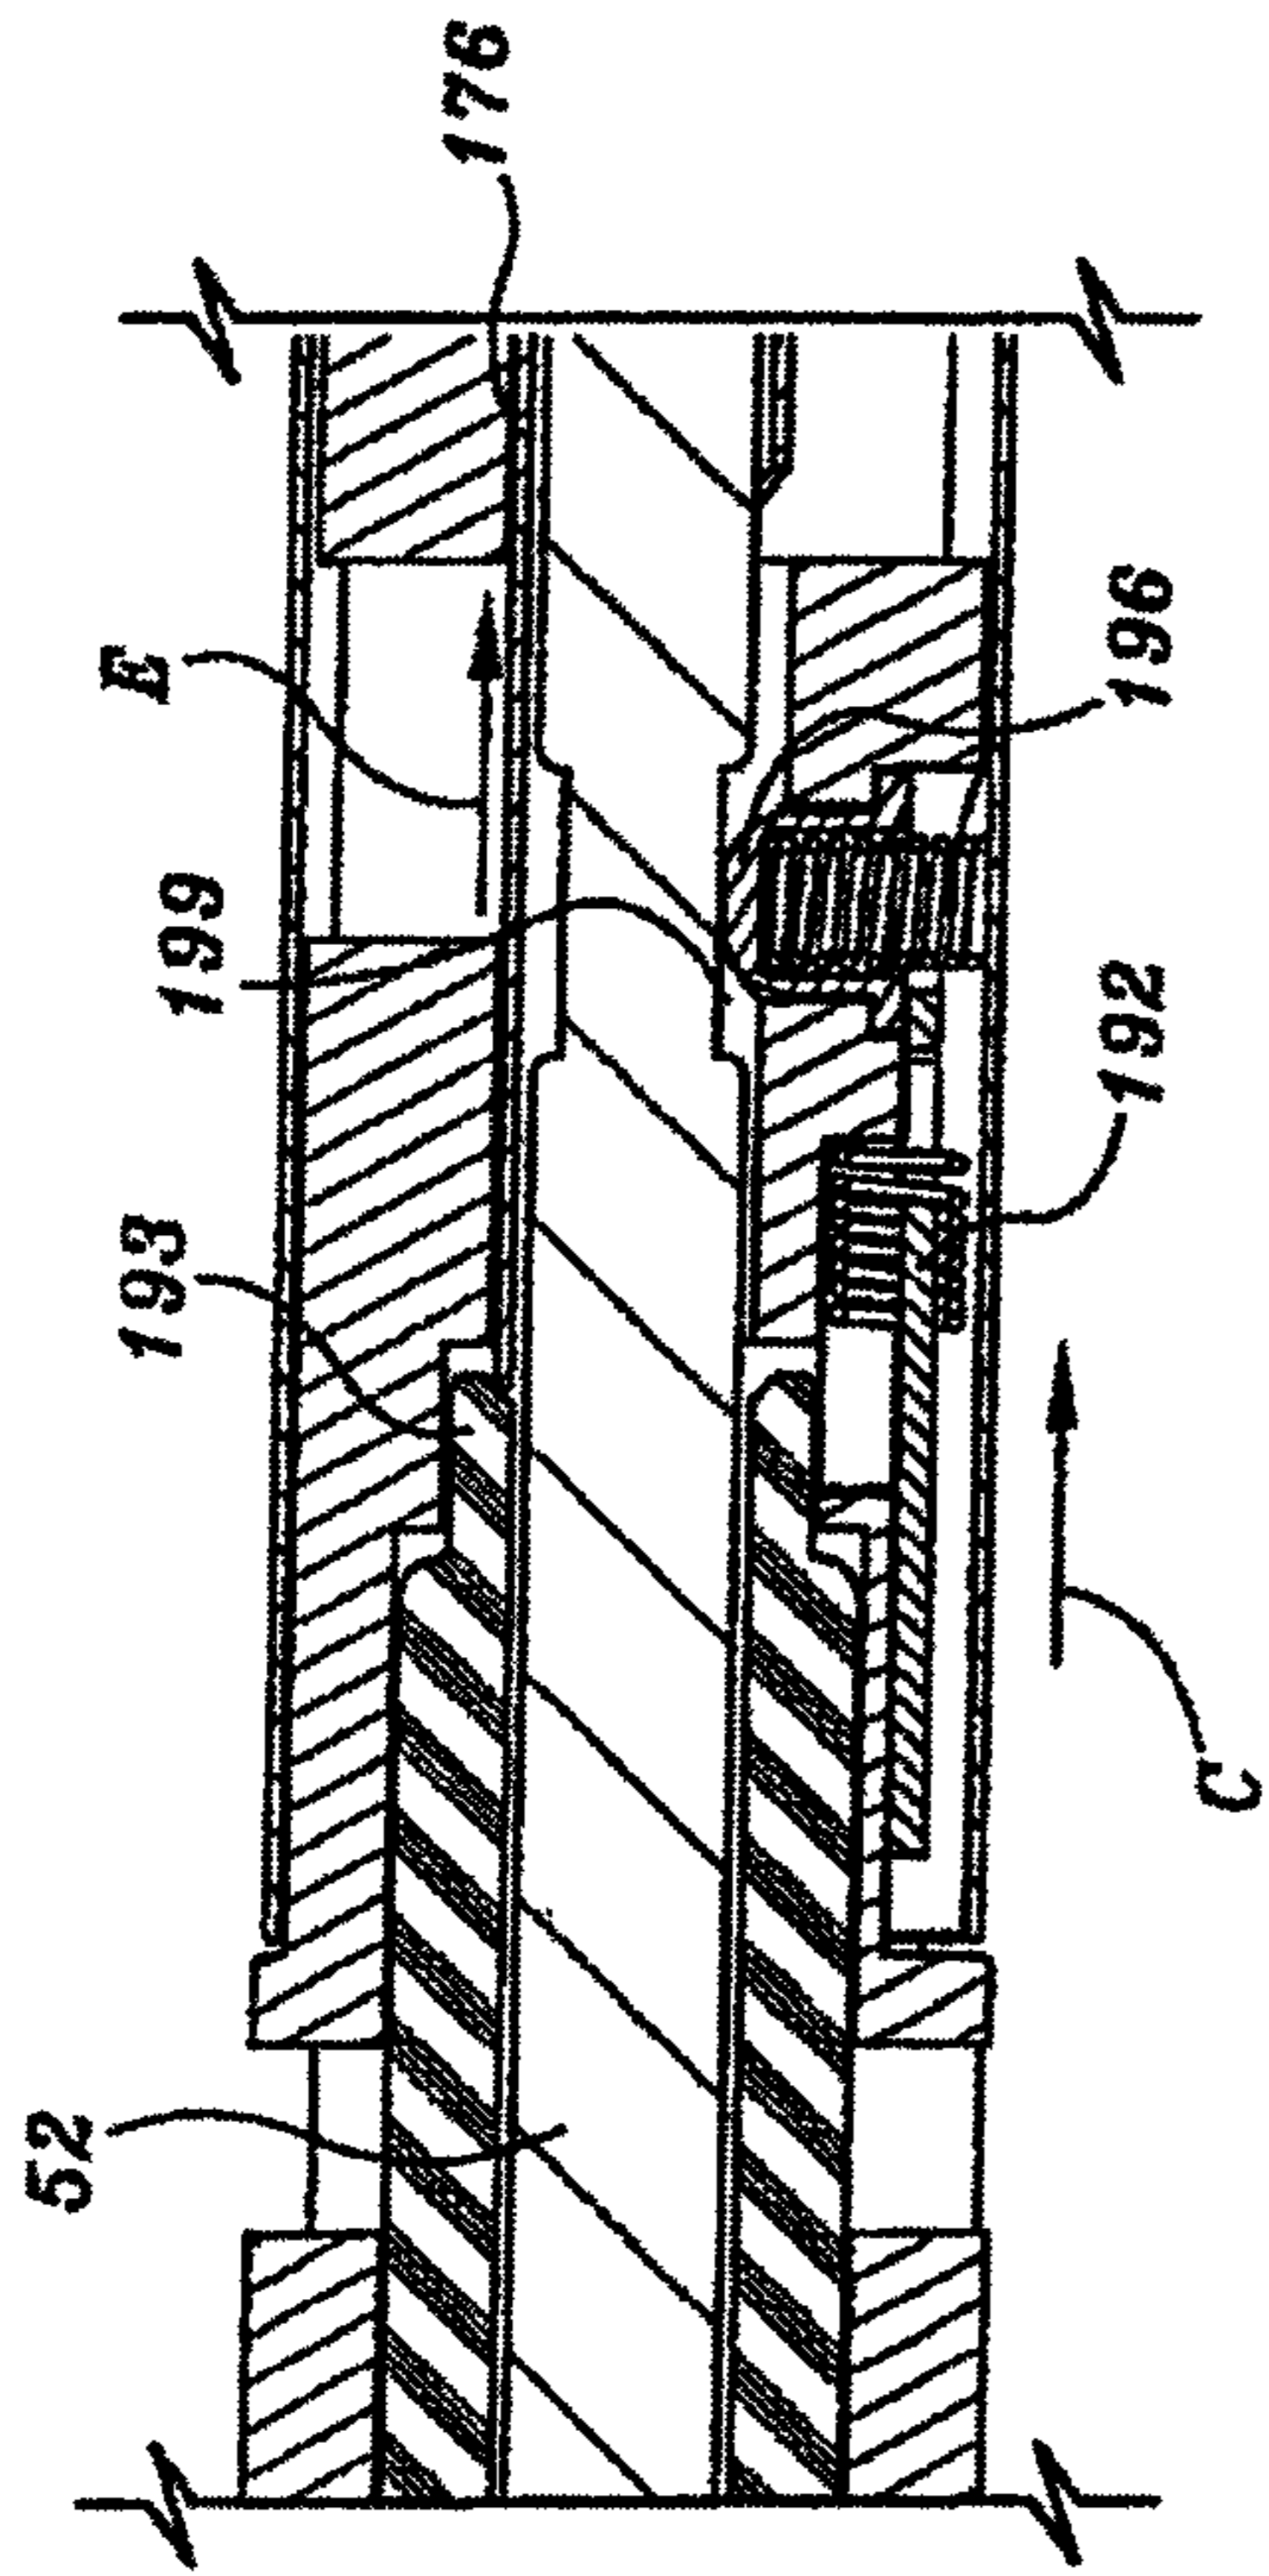


FIG. 43

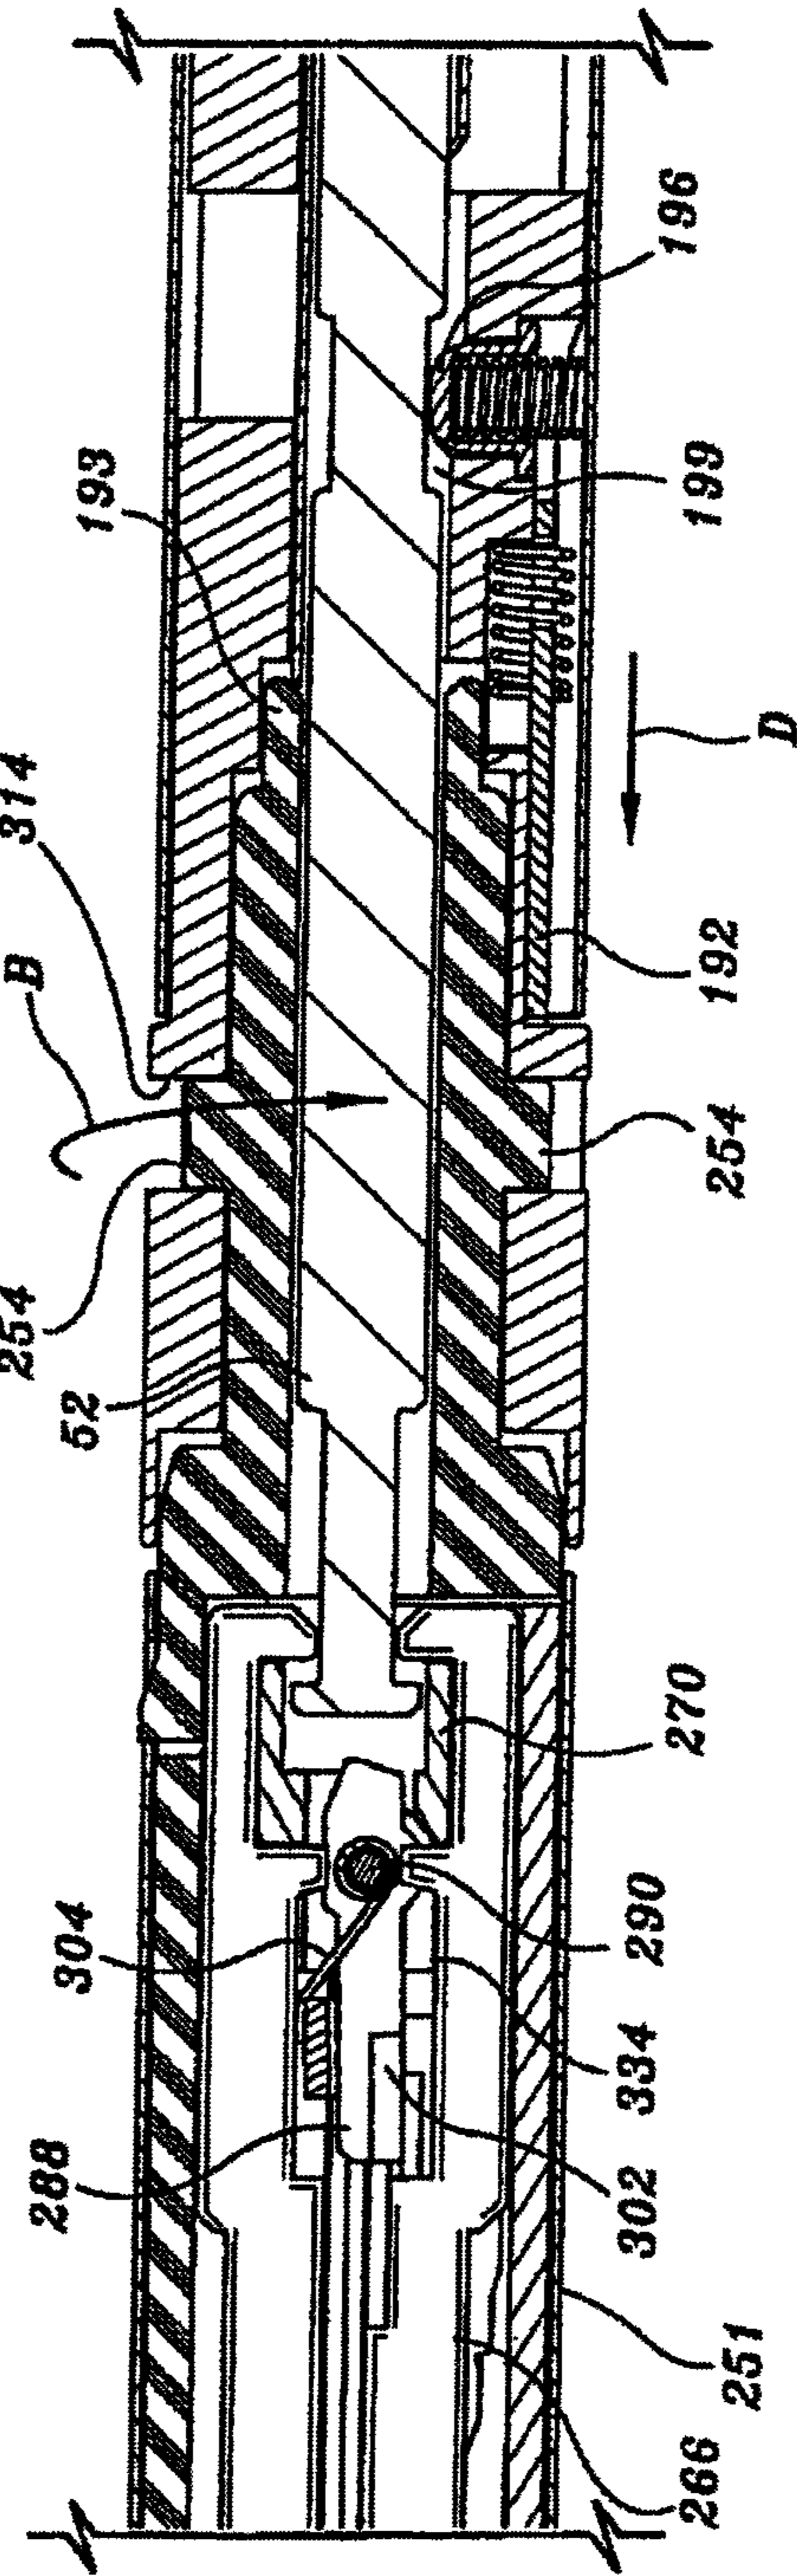


FIG. 44

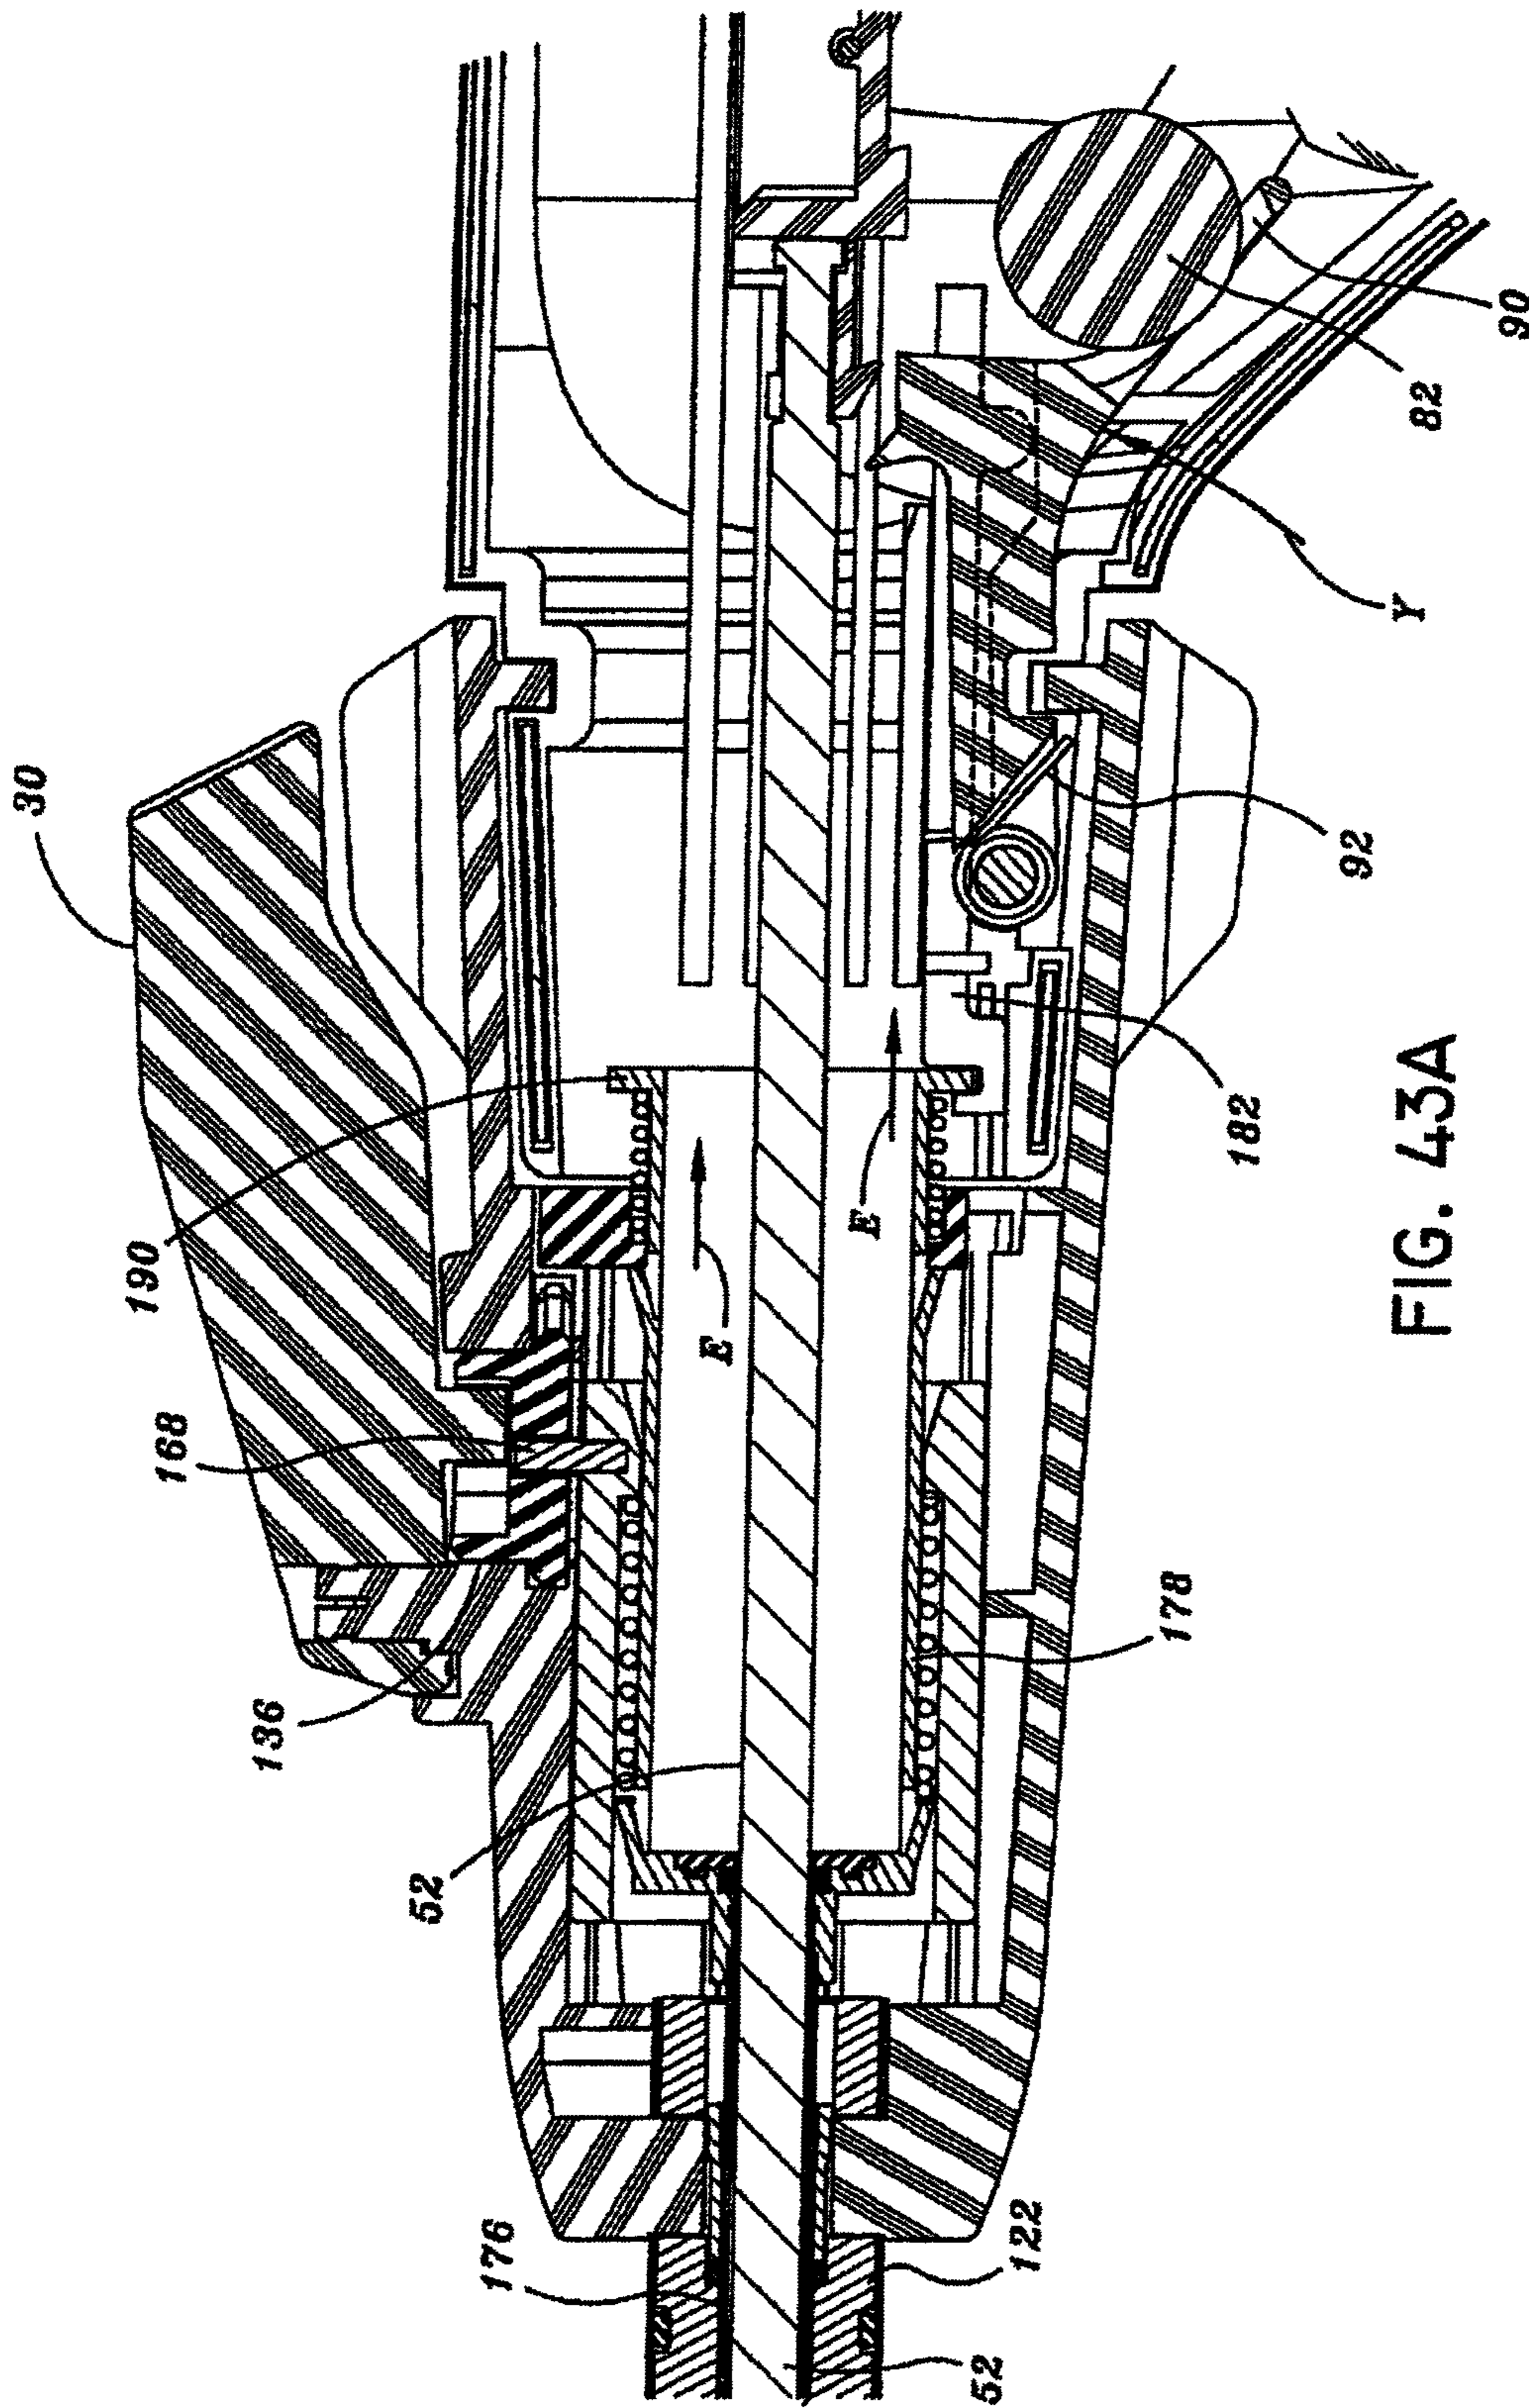


FIG. 43A

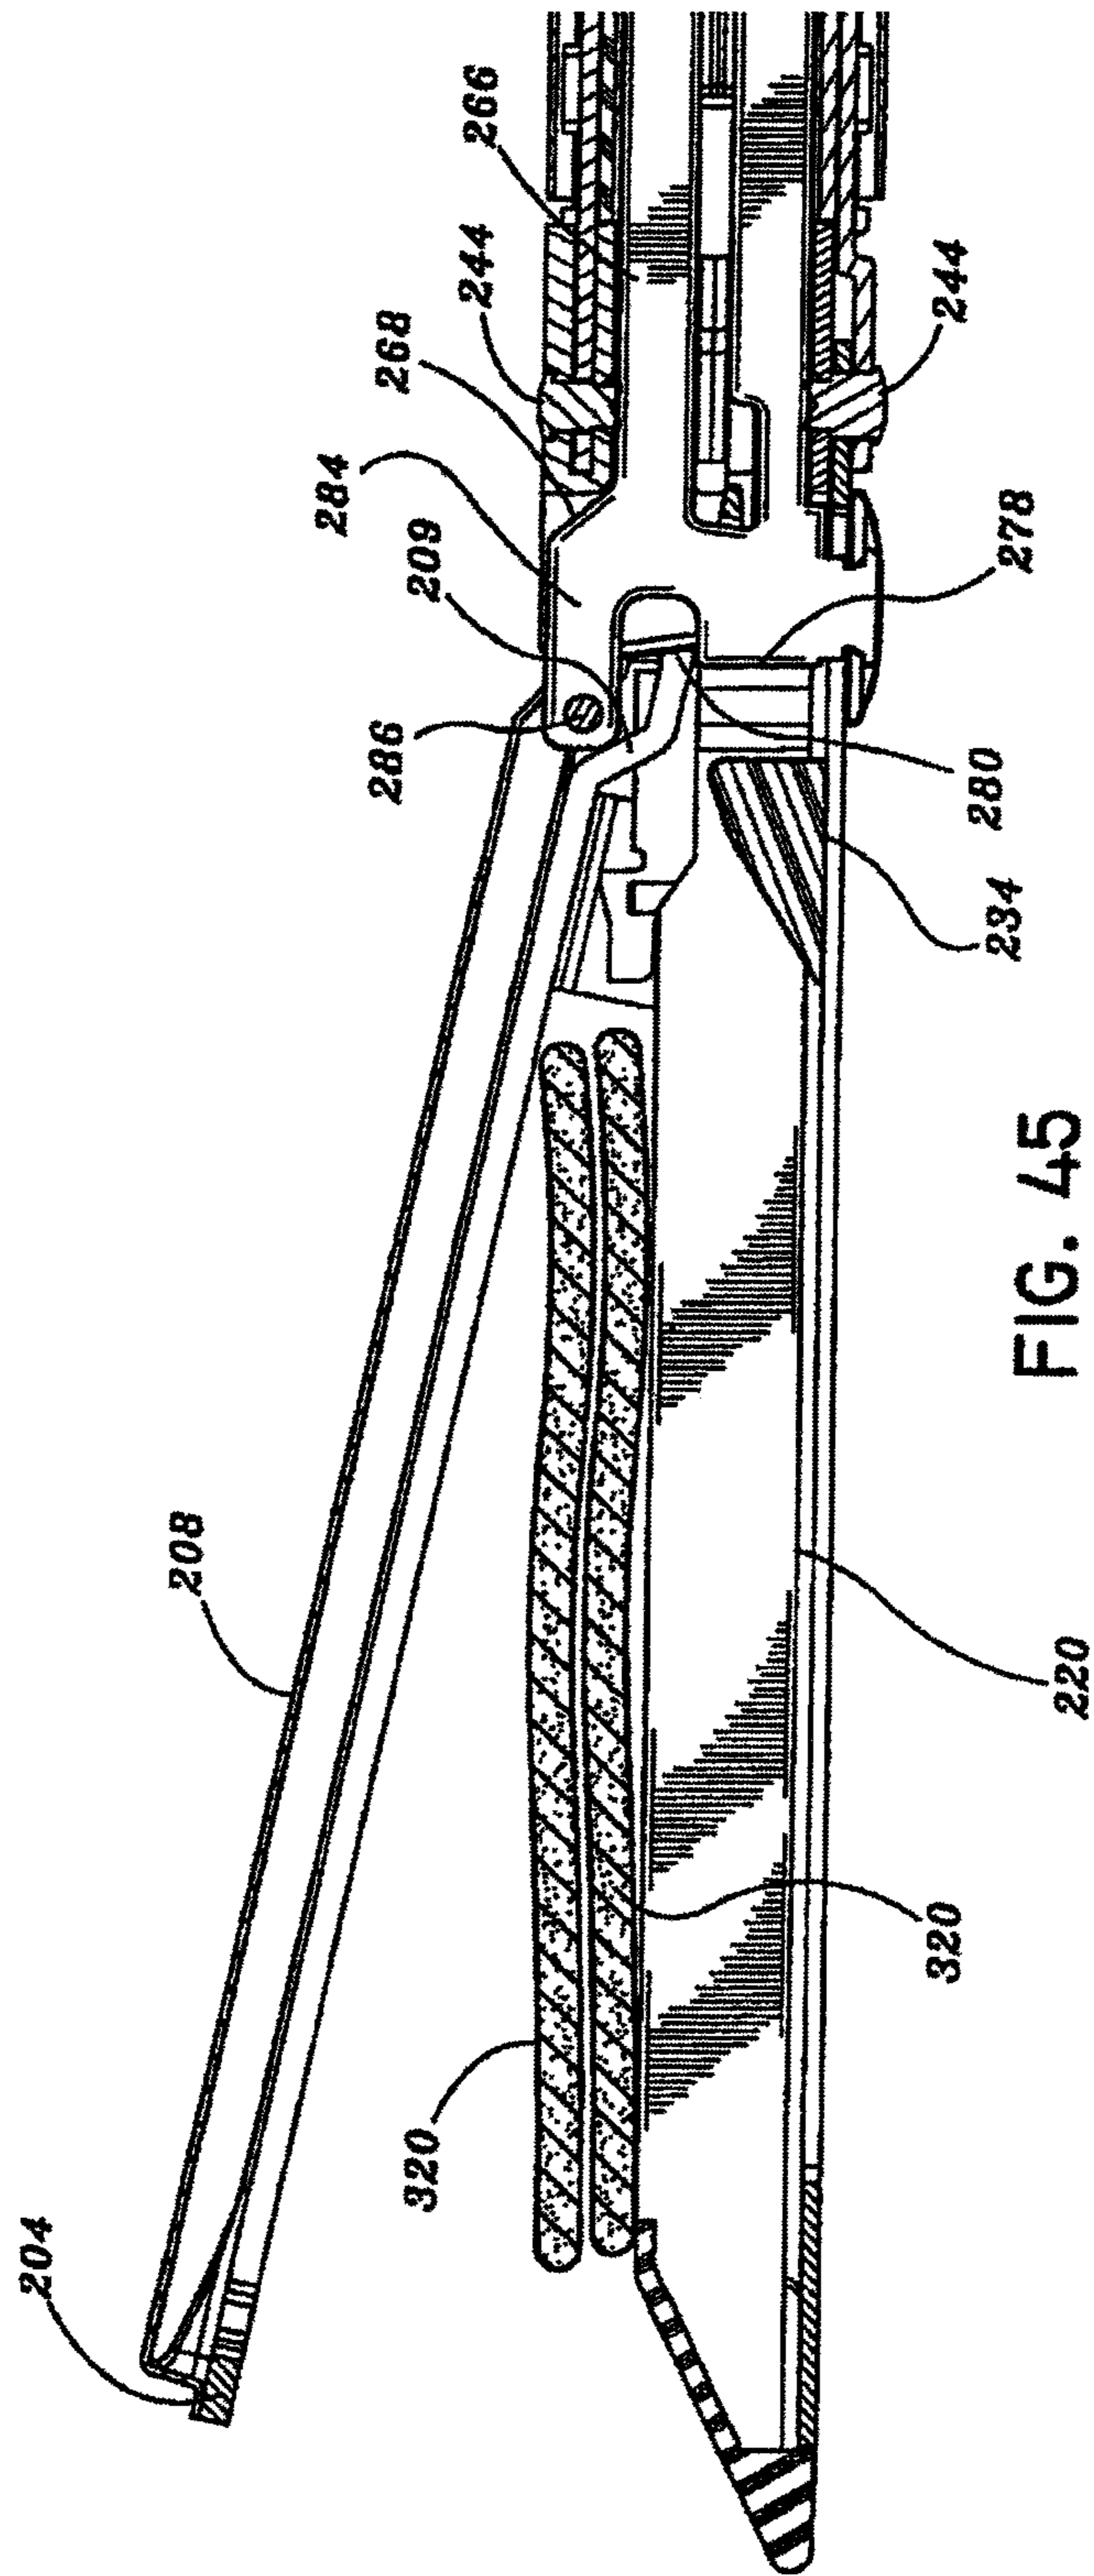


FIG. 45

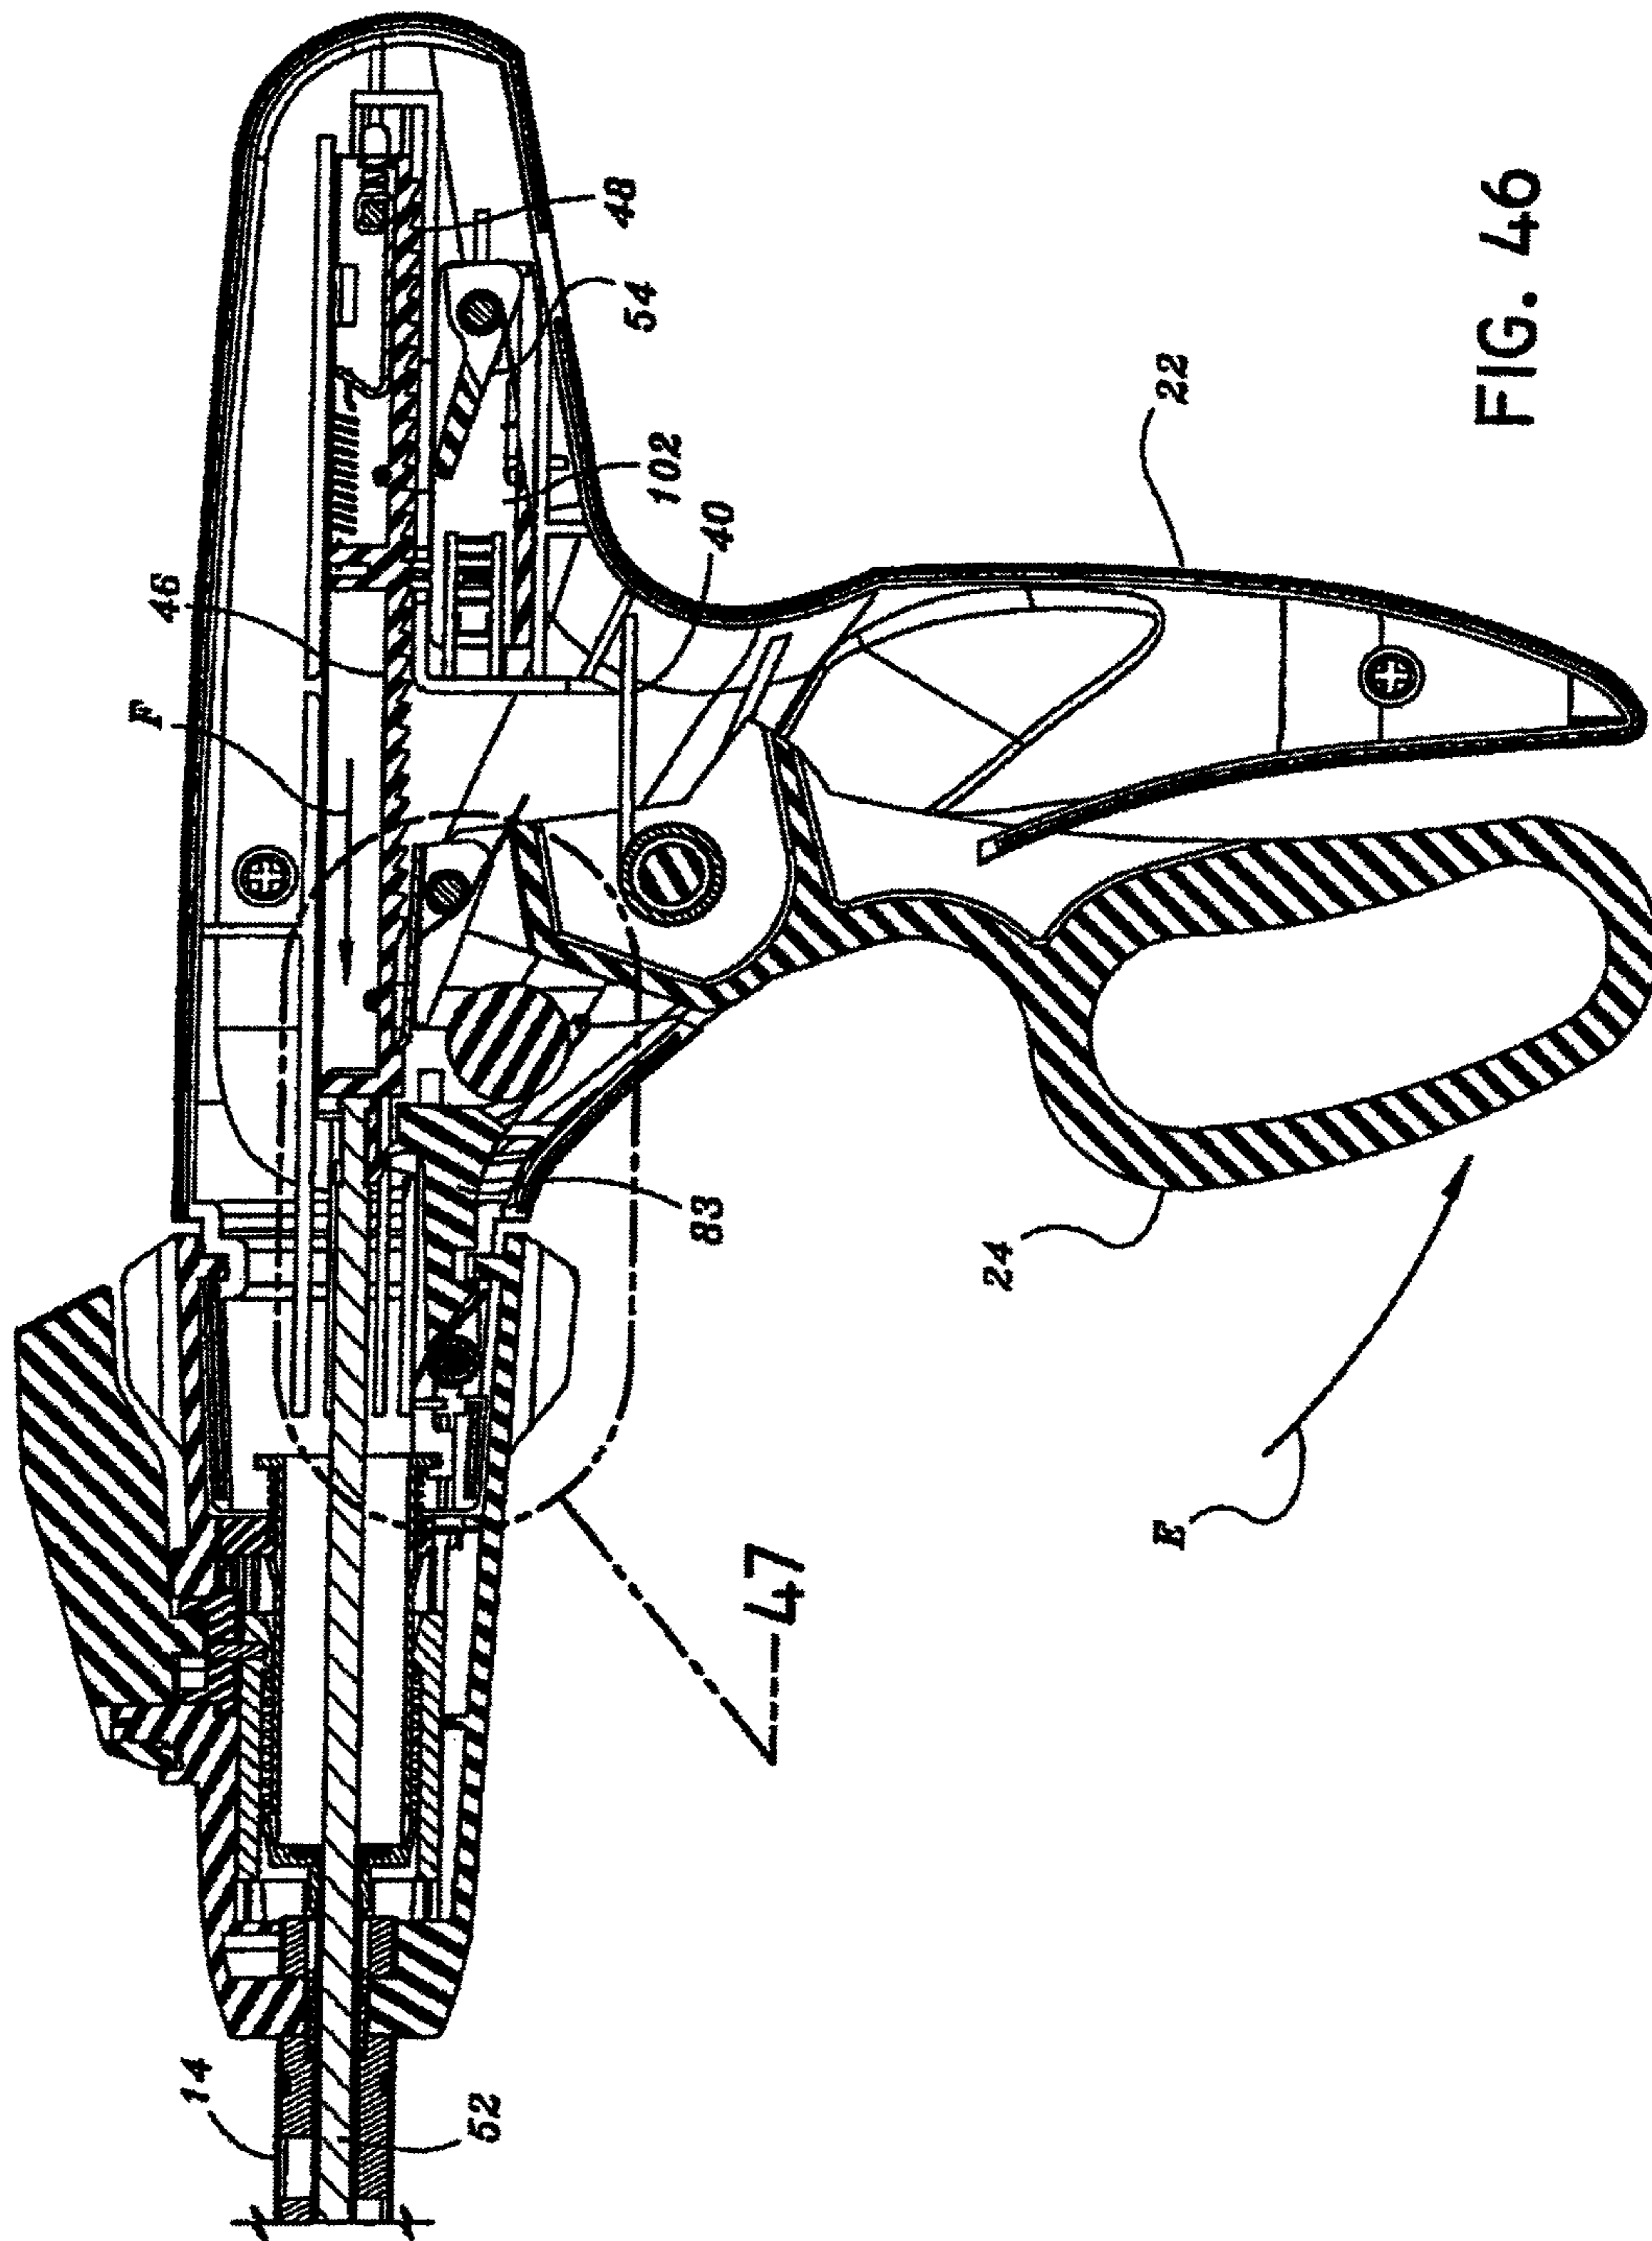
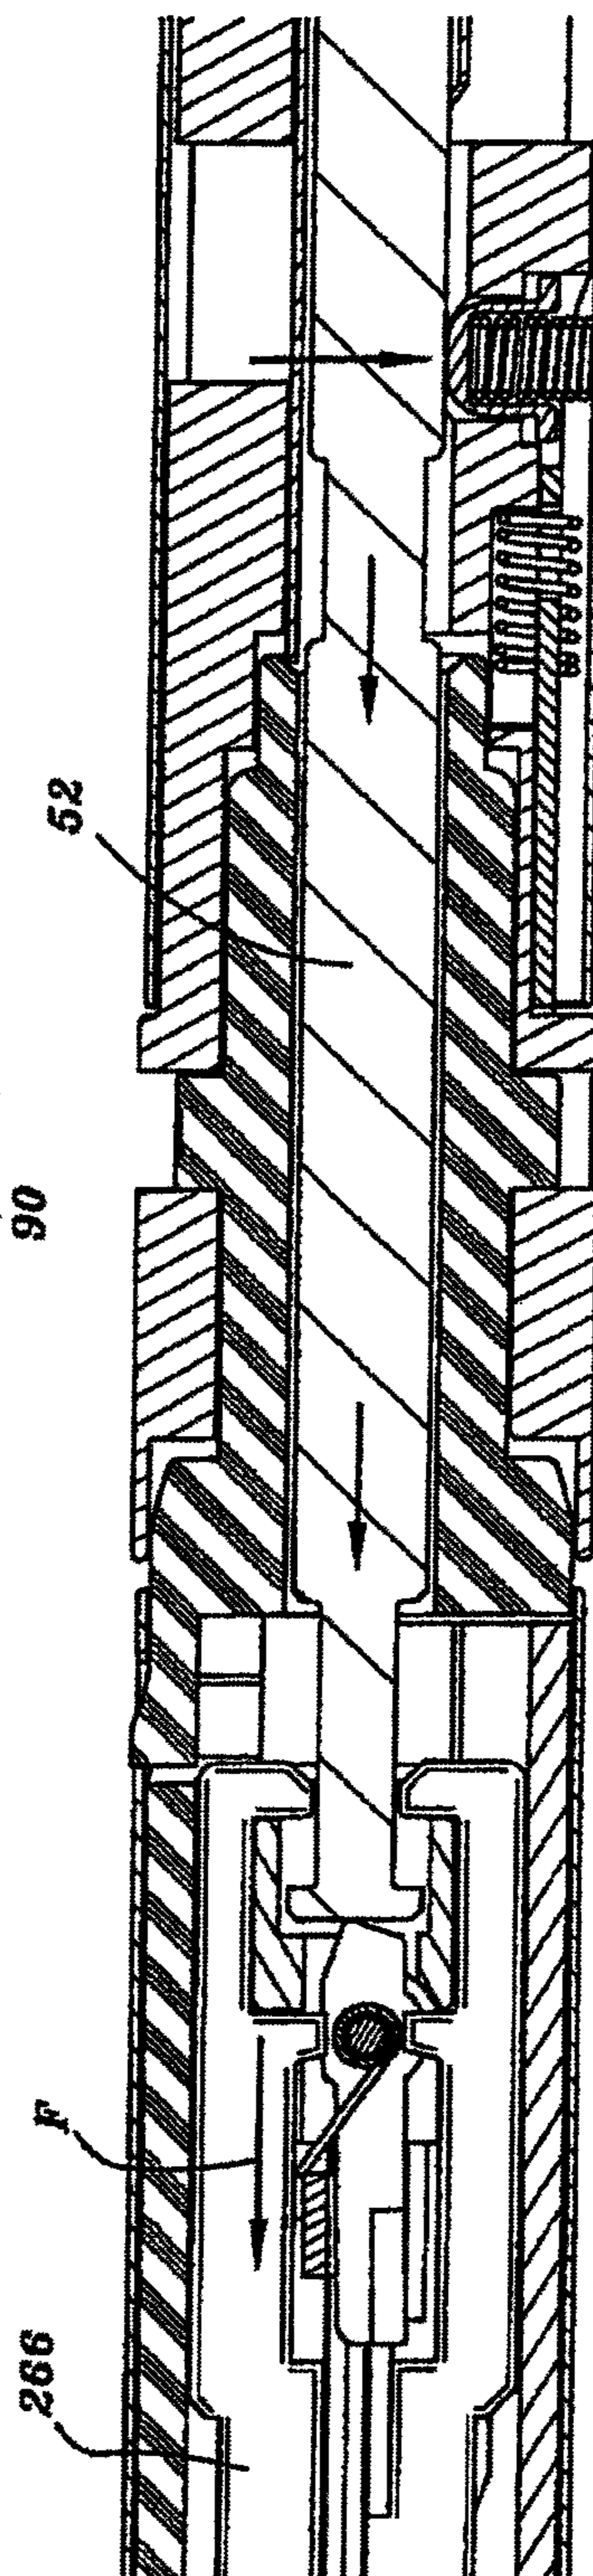
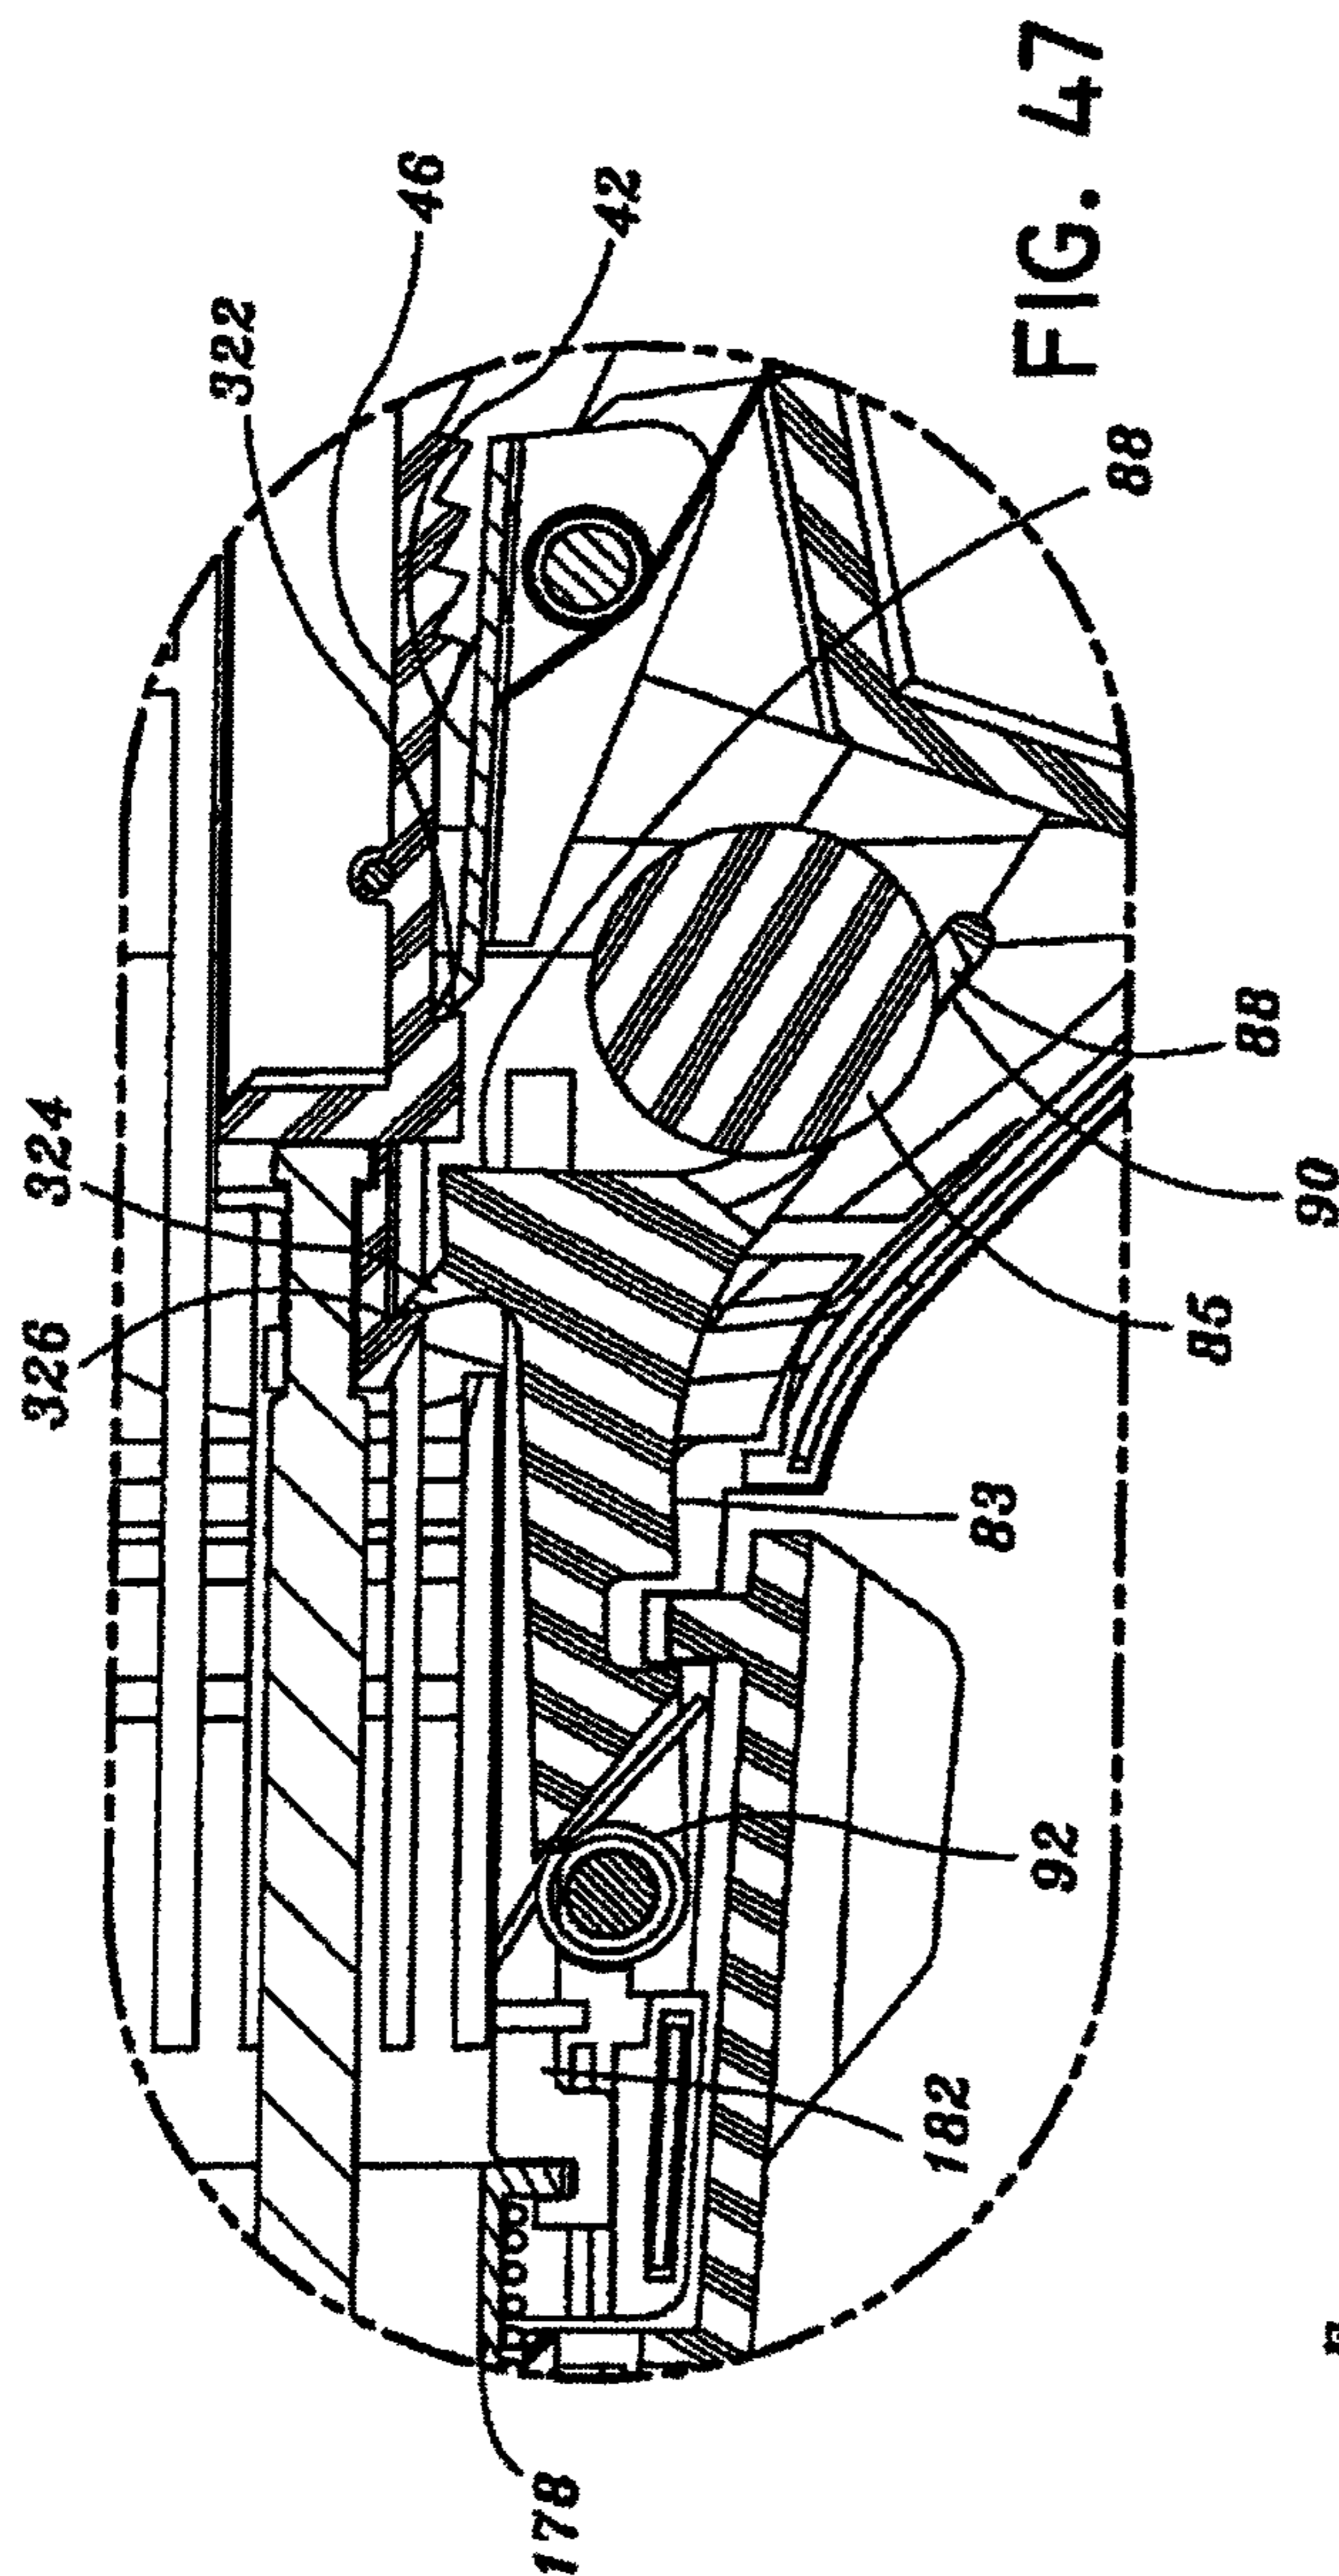


FIG. 46



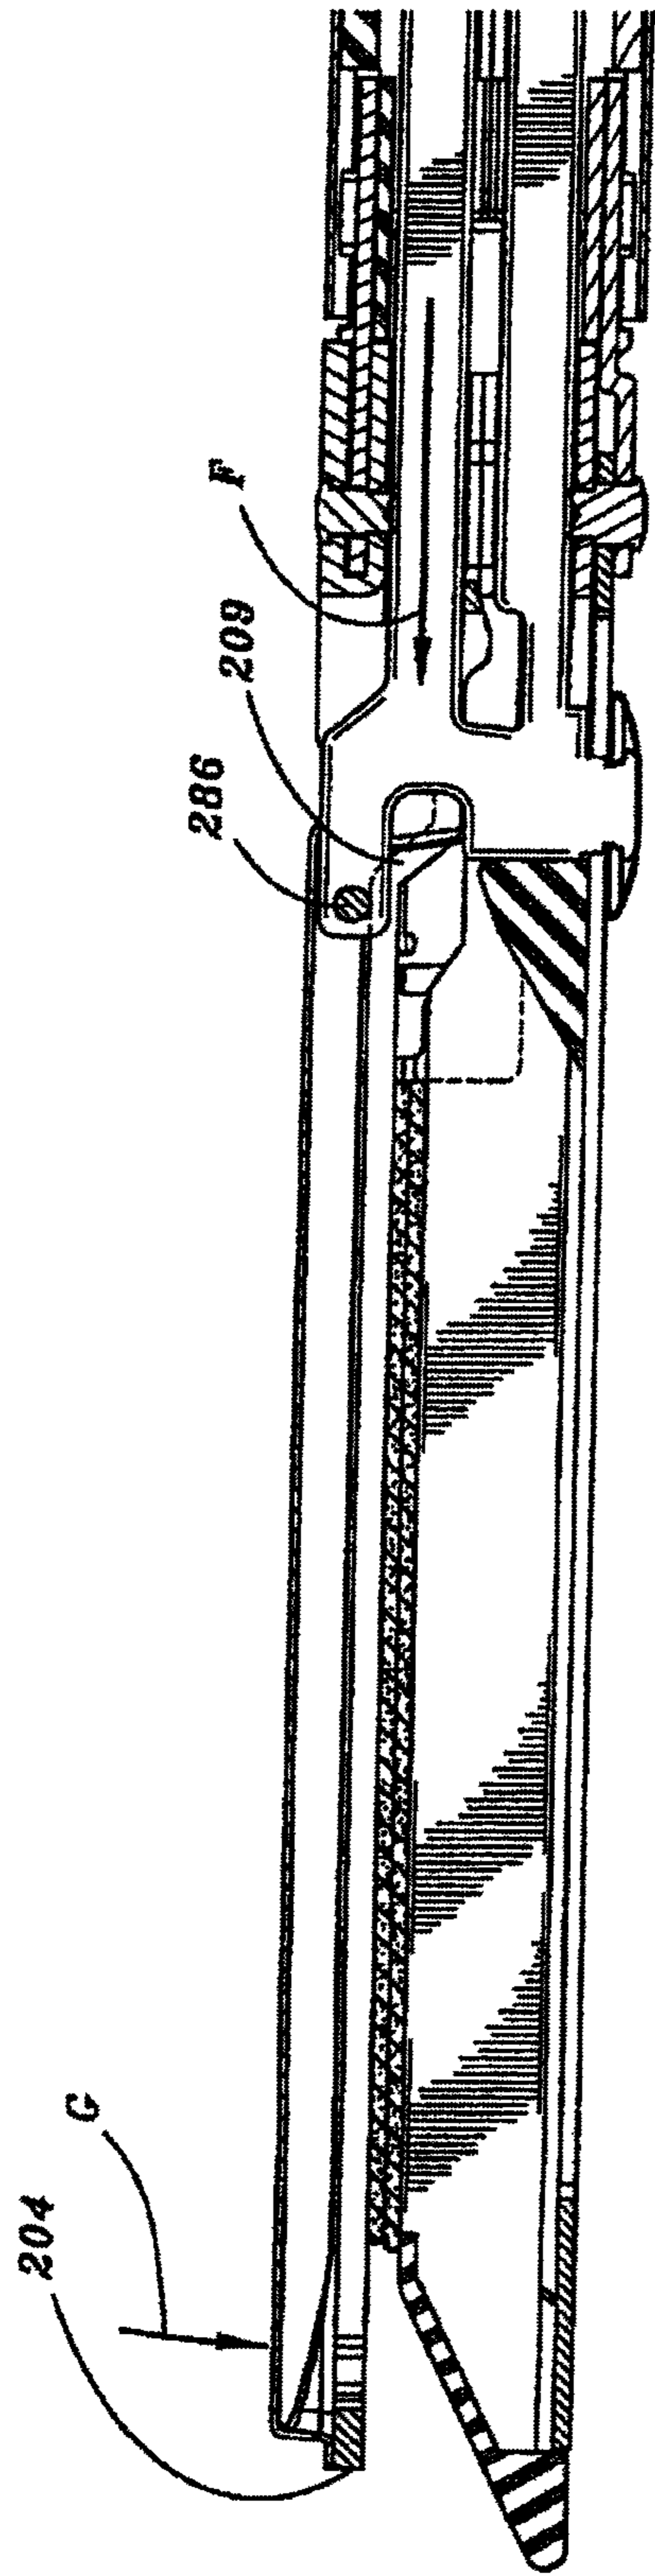


FIG. 49



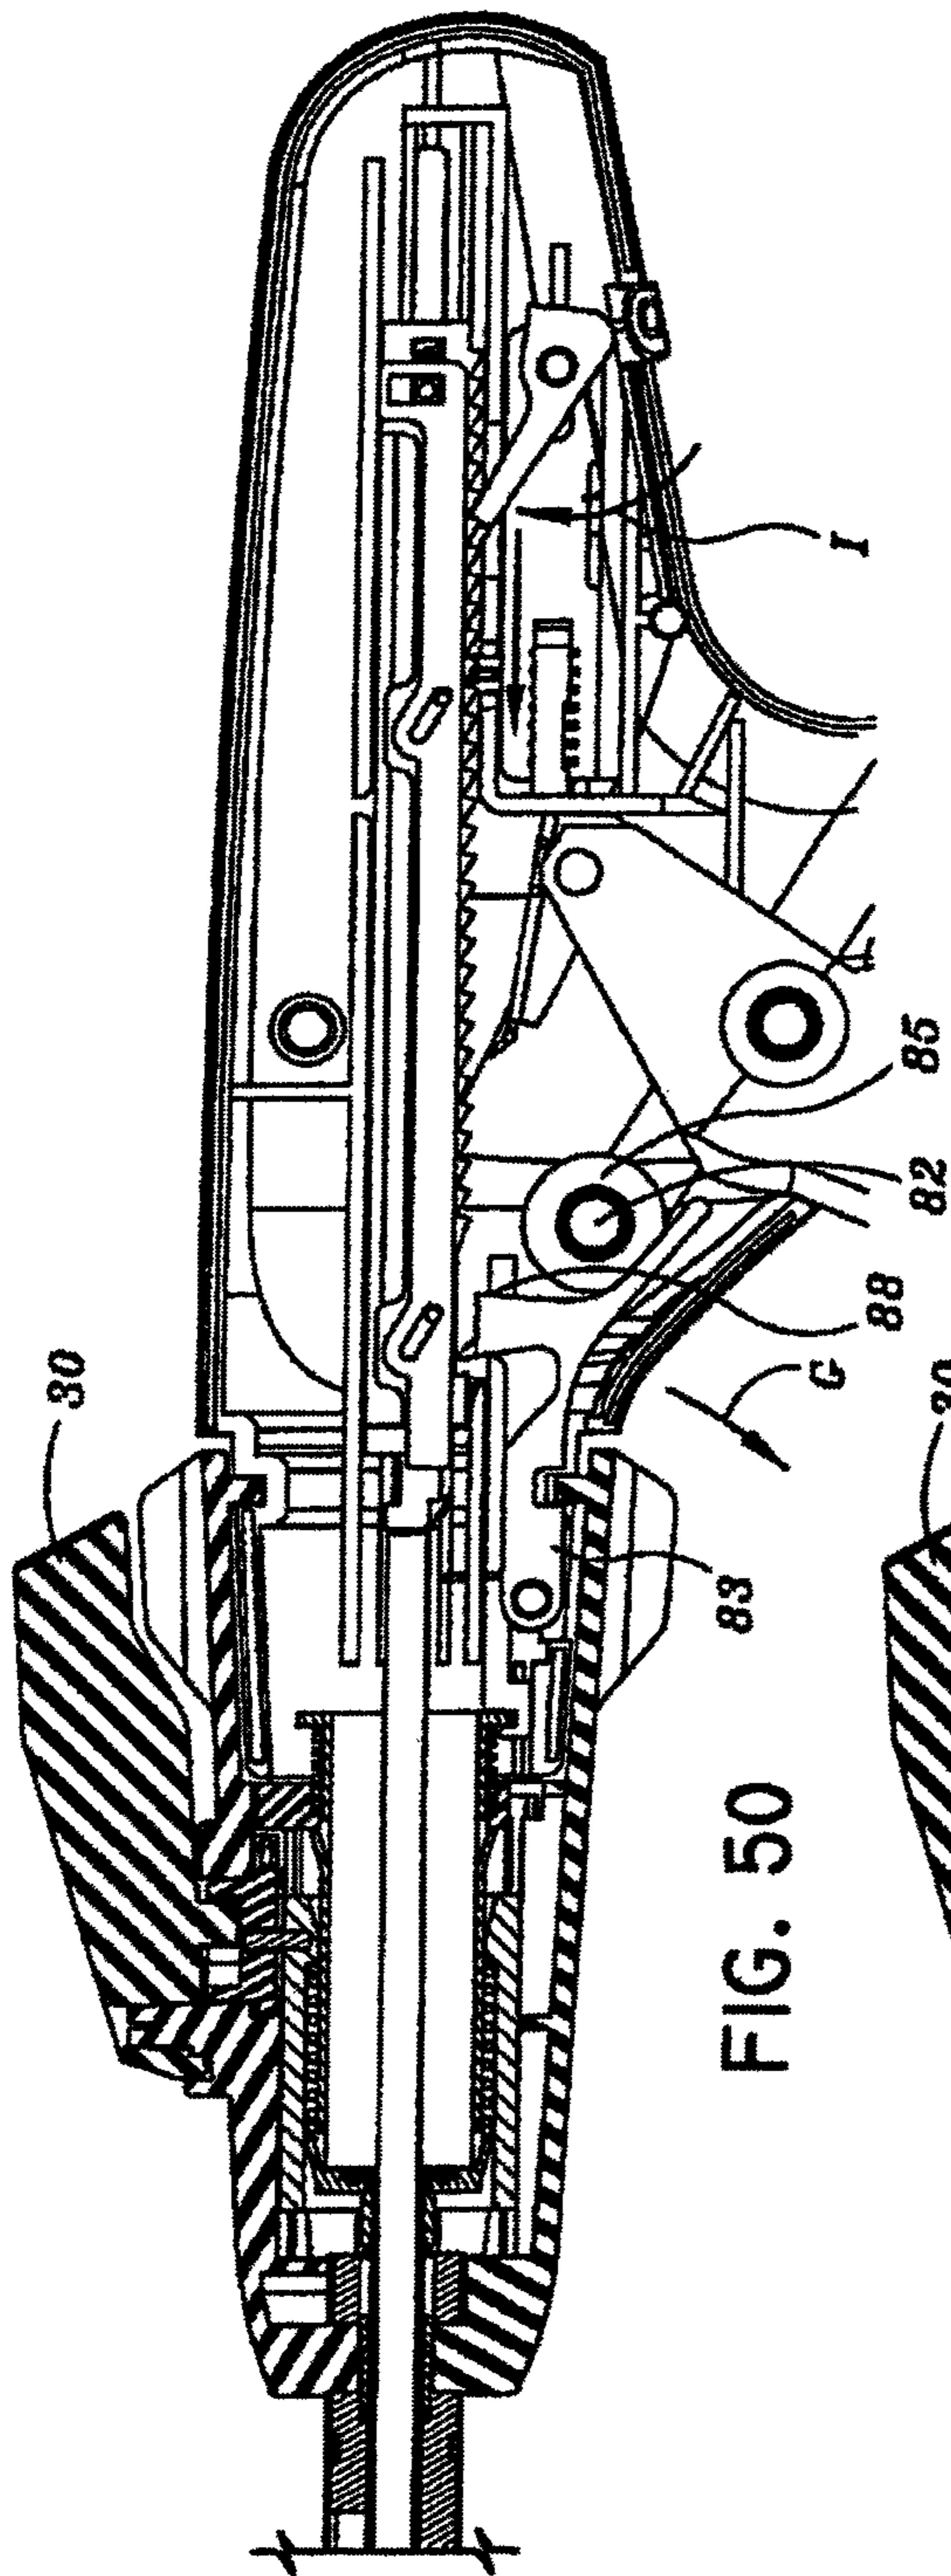


FIG. 50

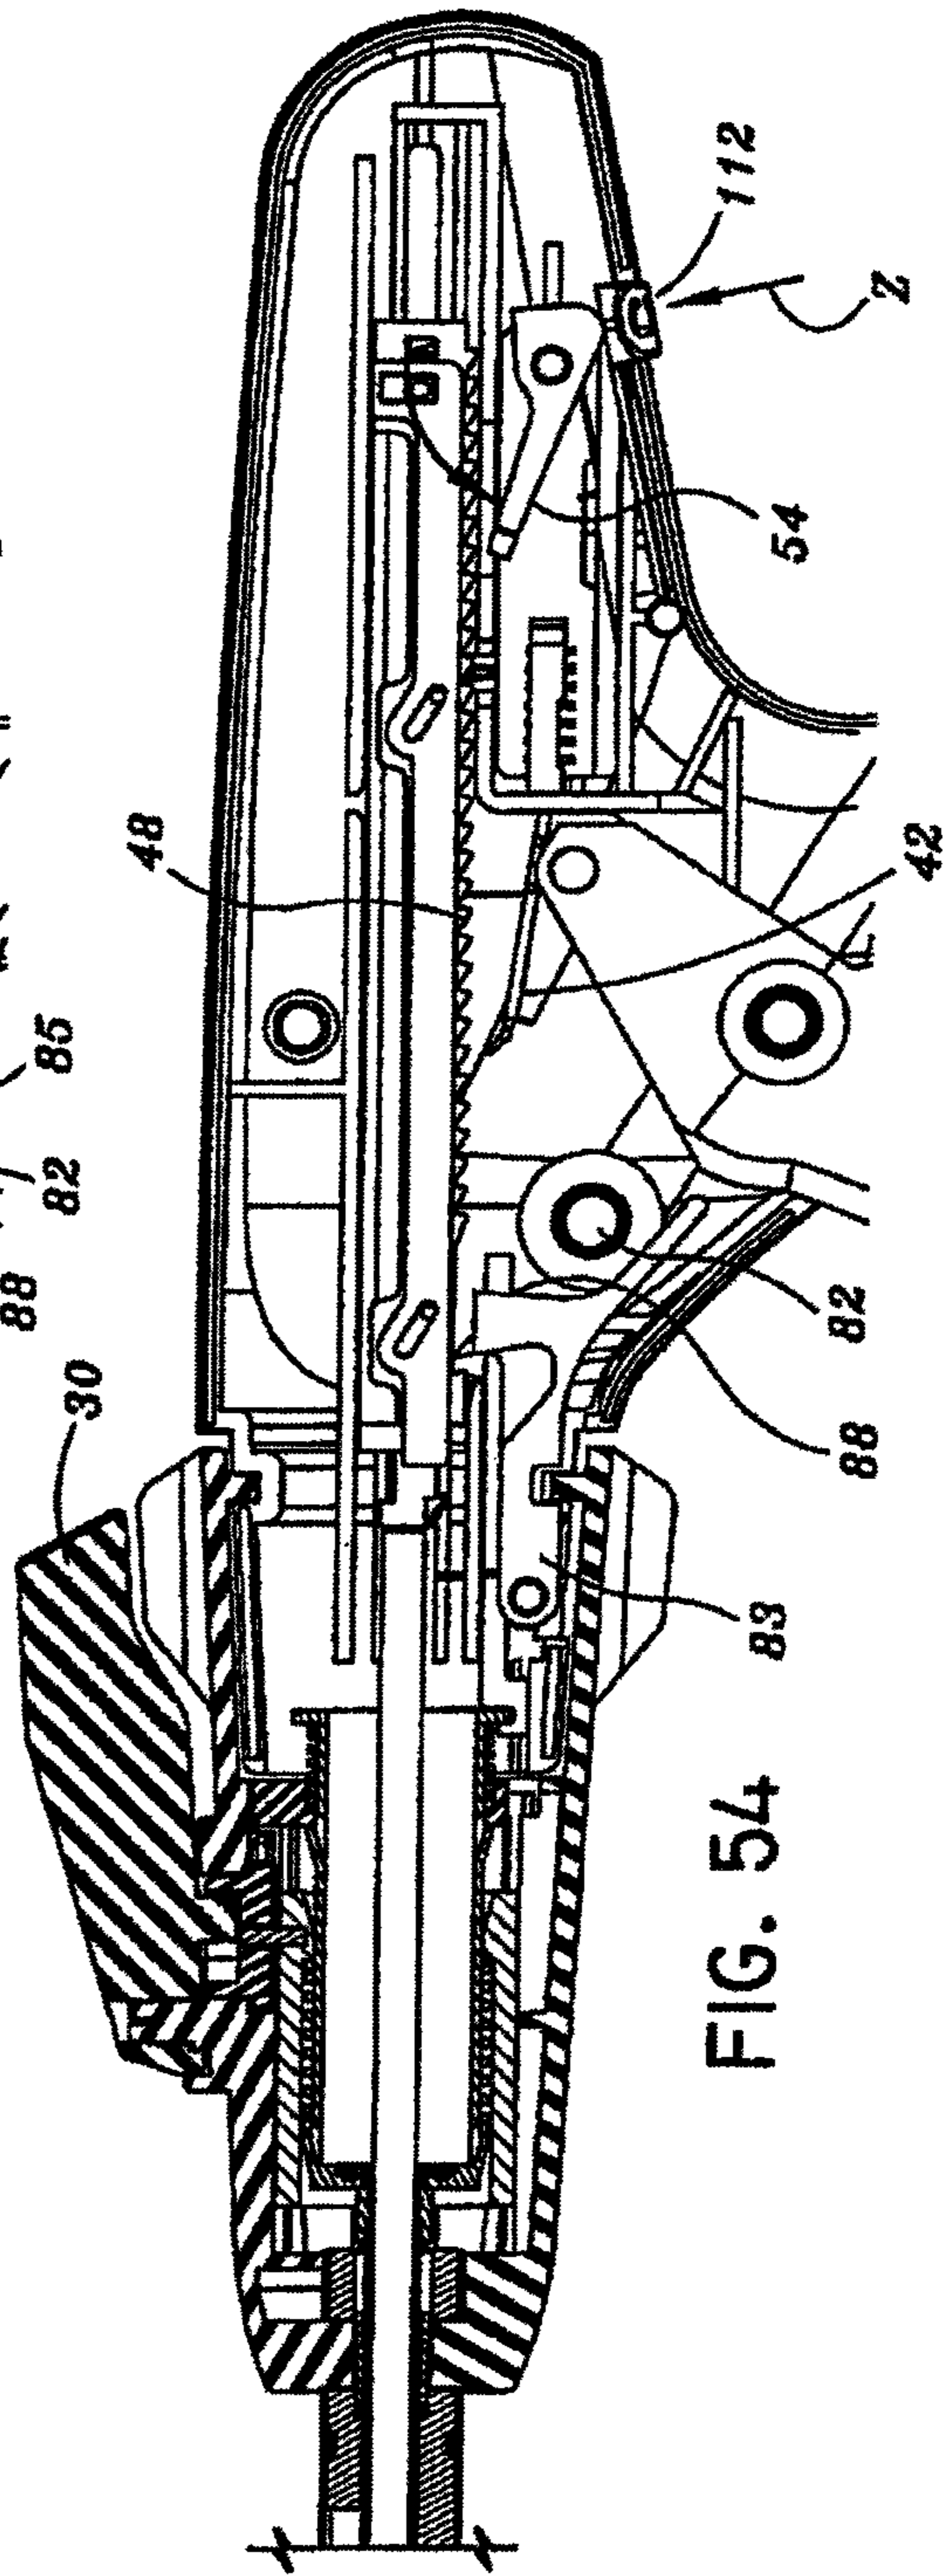


FIG. 54

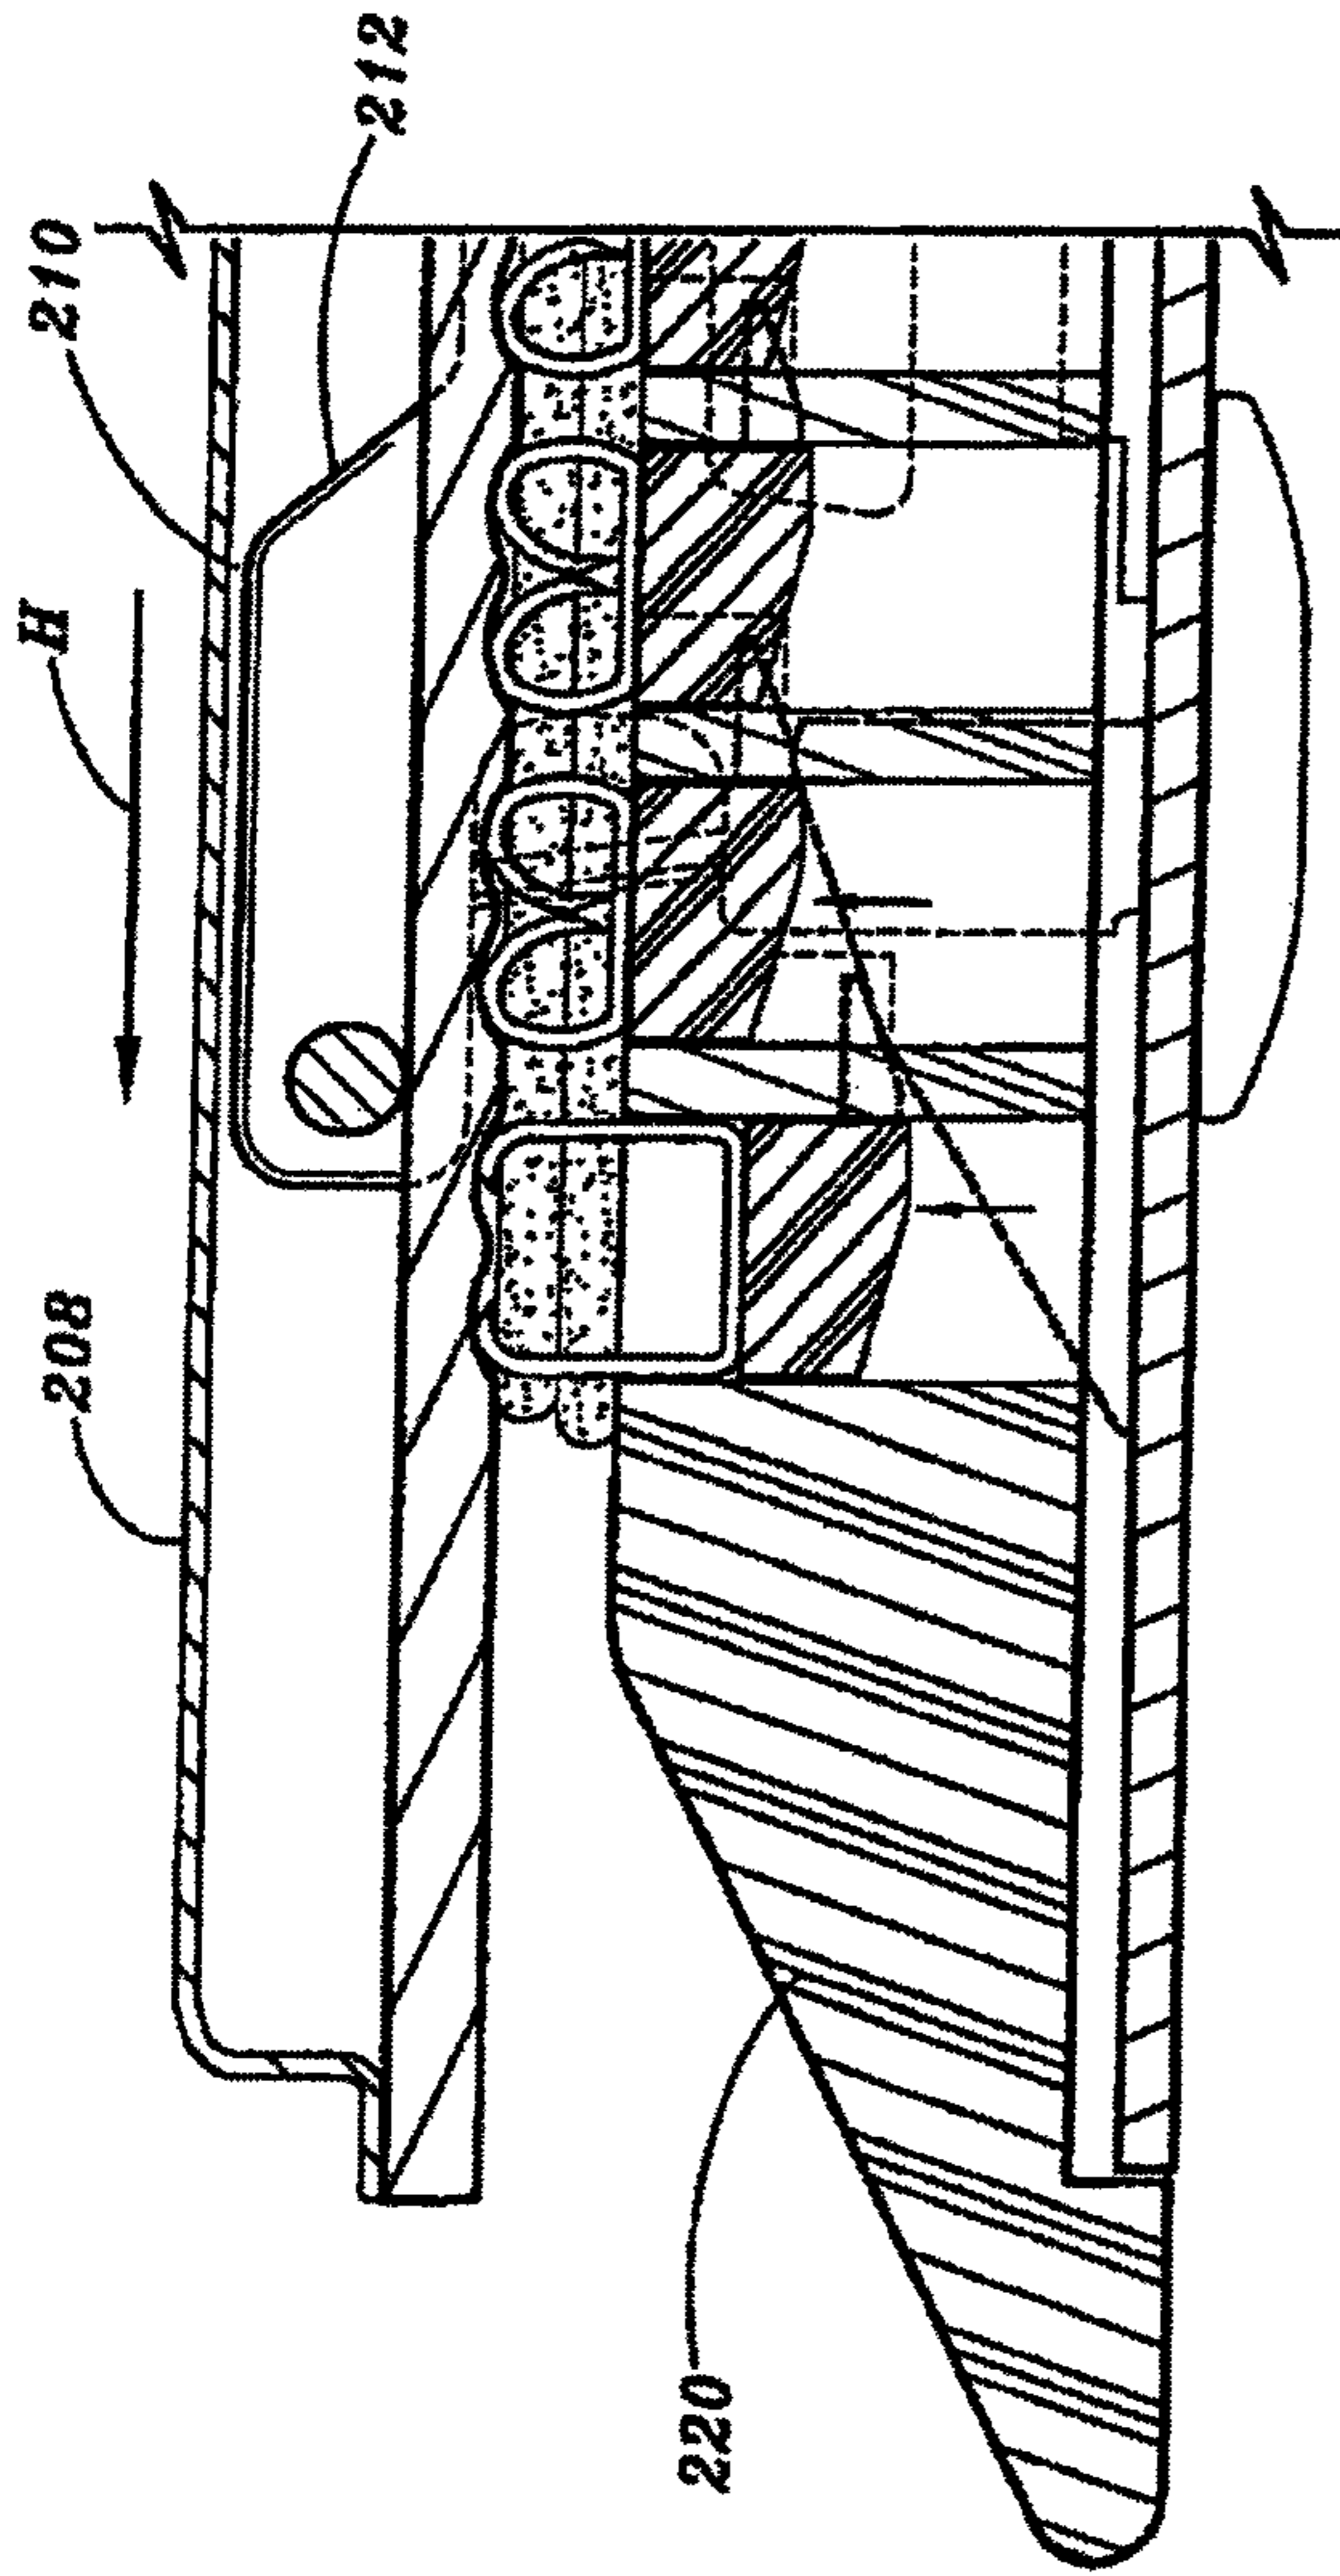


FIG. 51

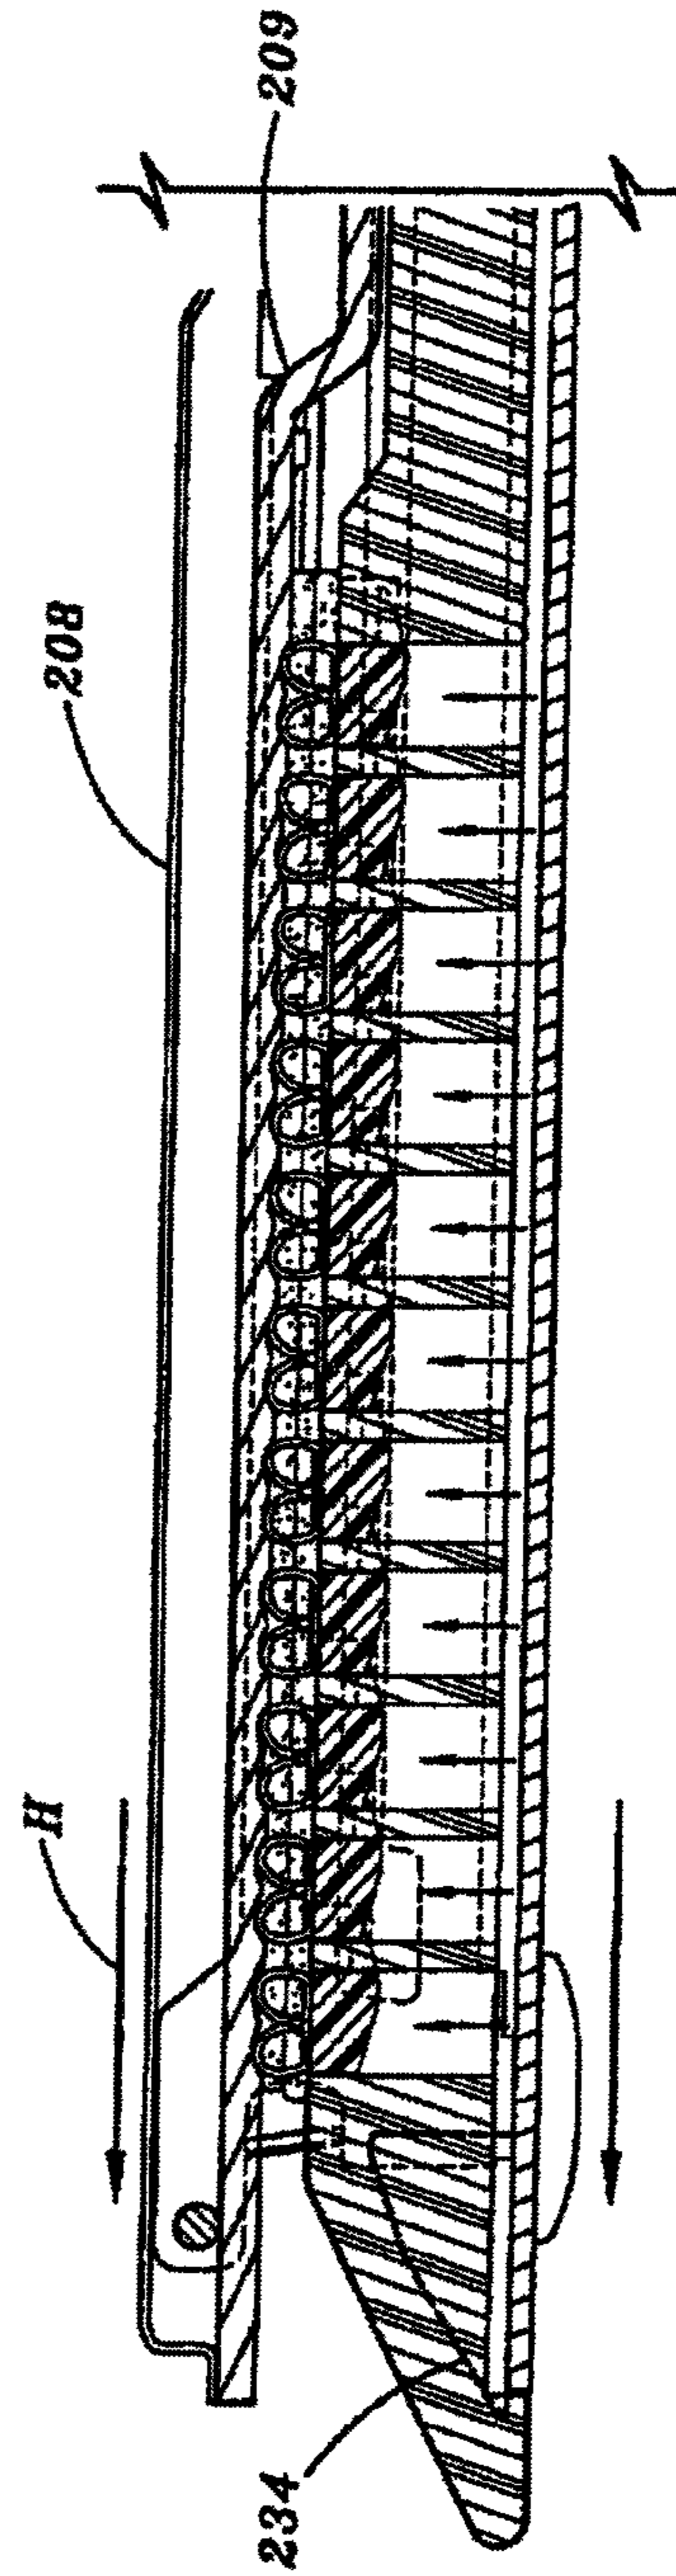


FIG. 52

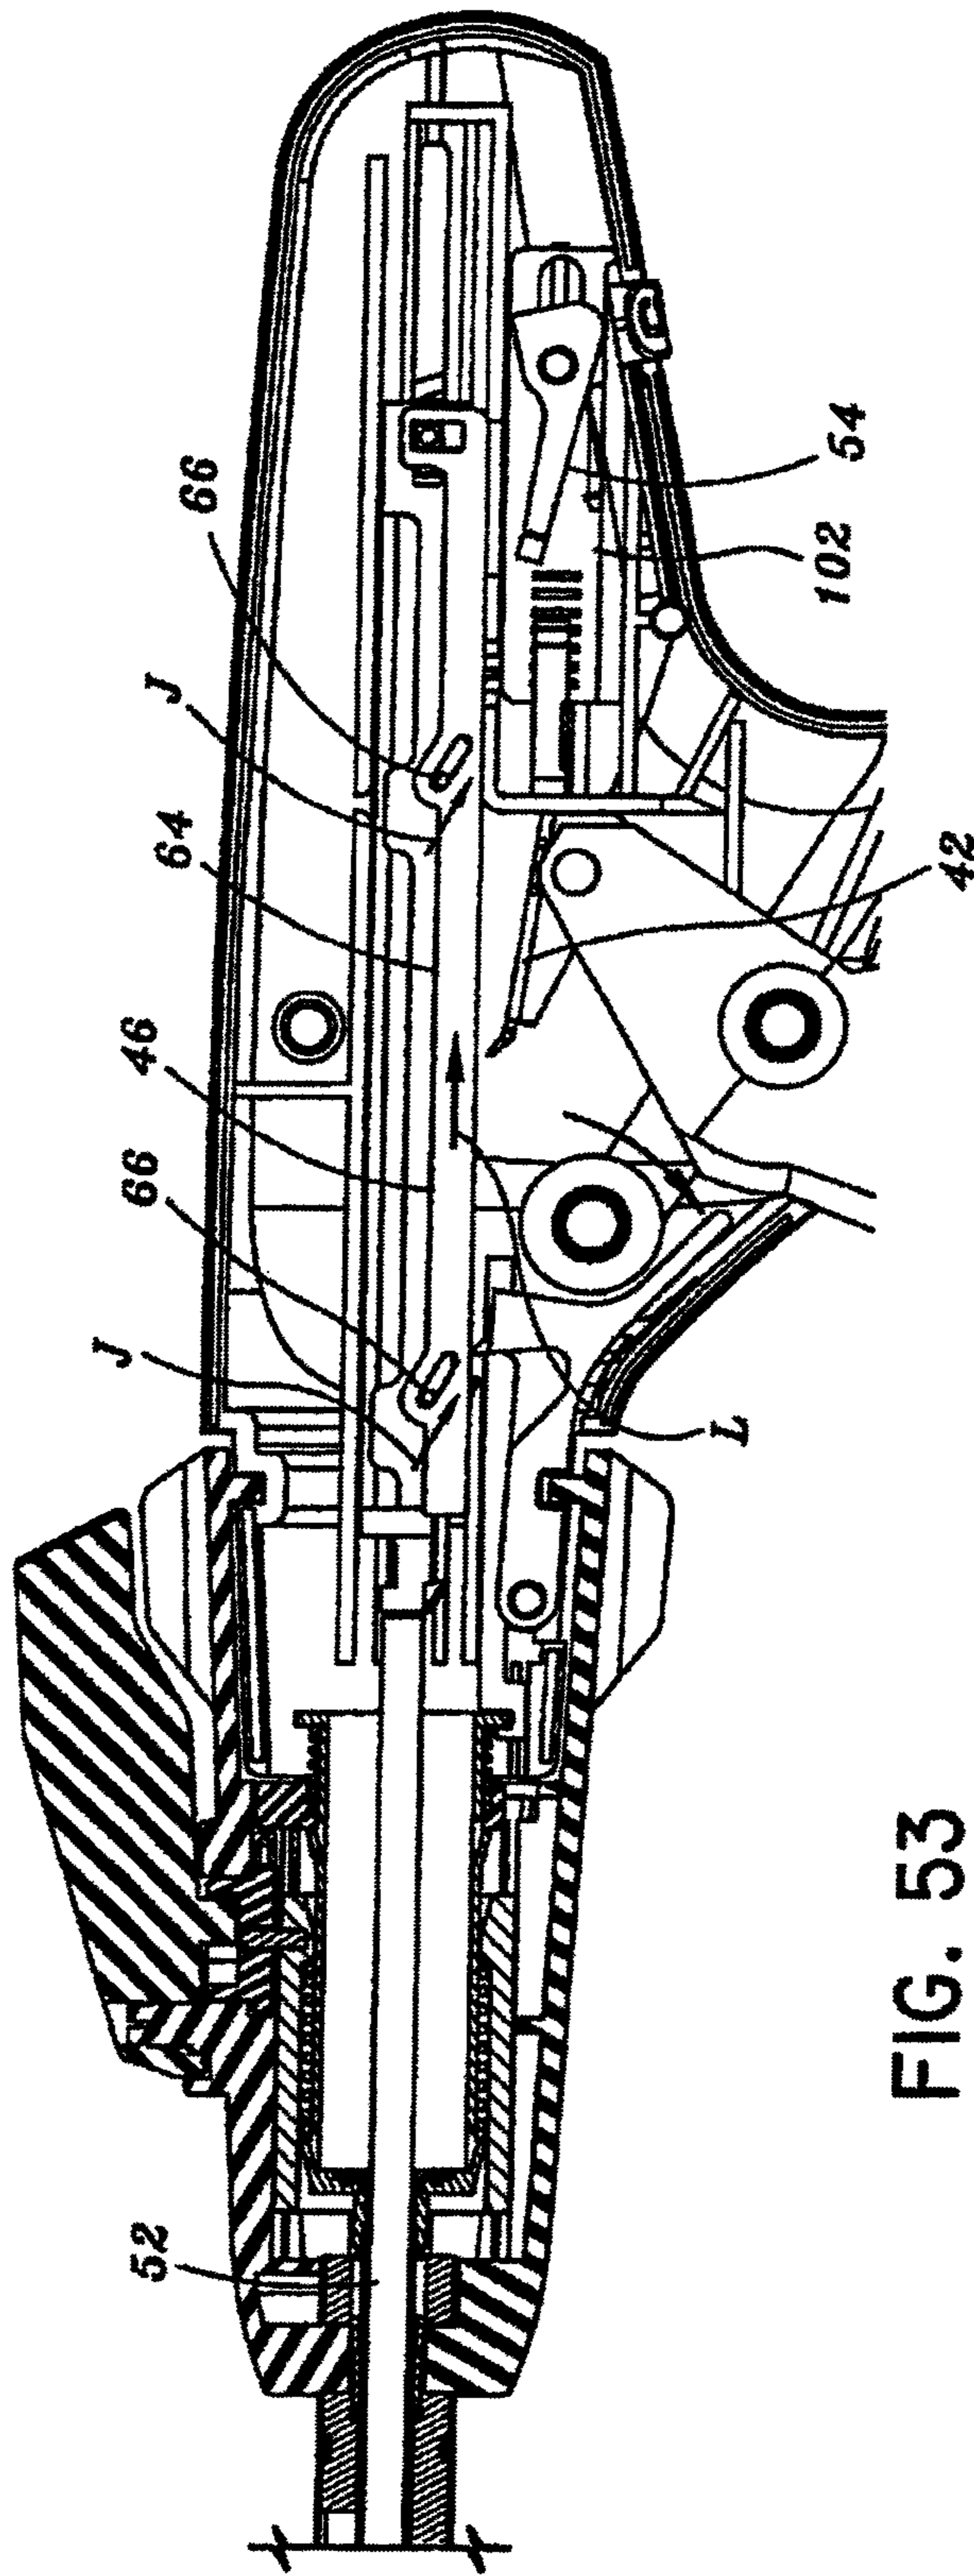


FIG. 53

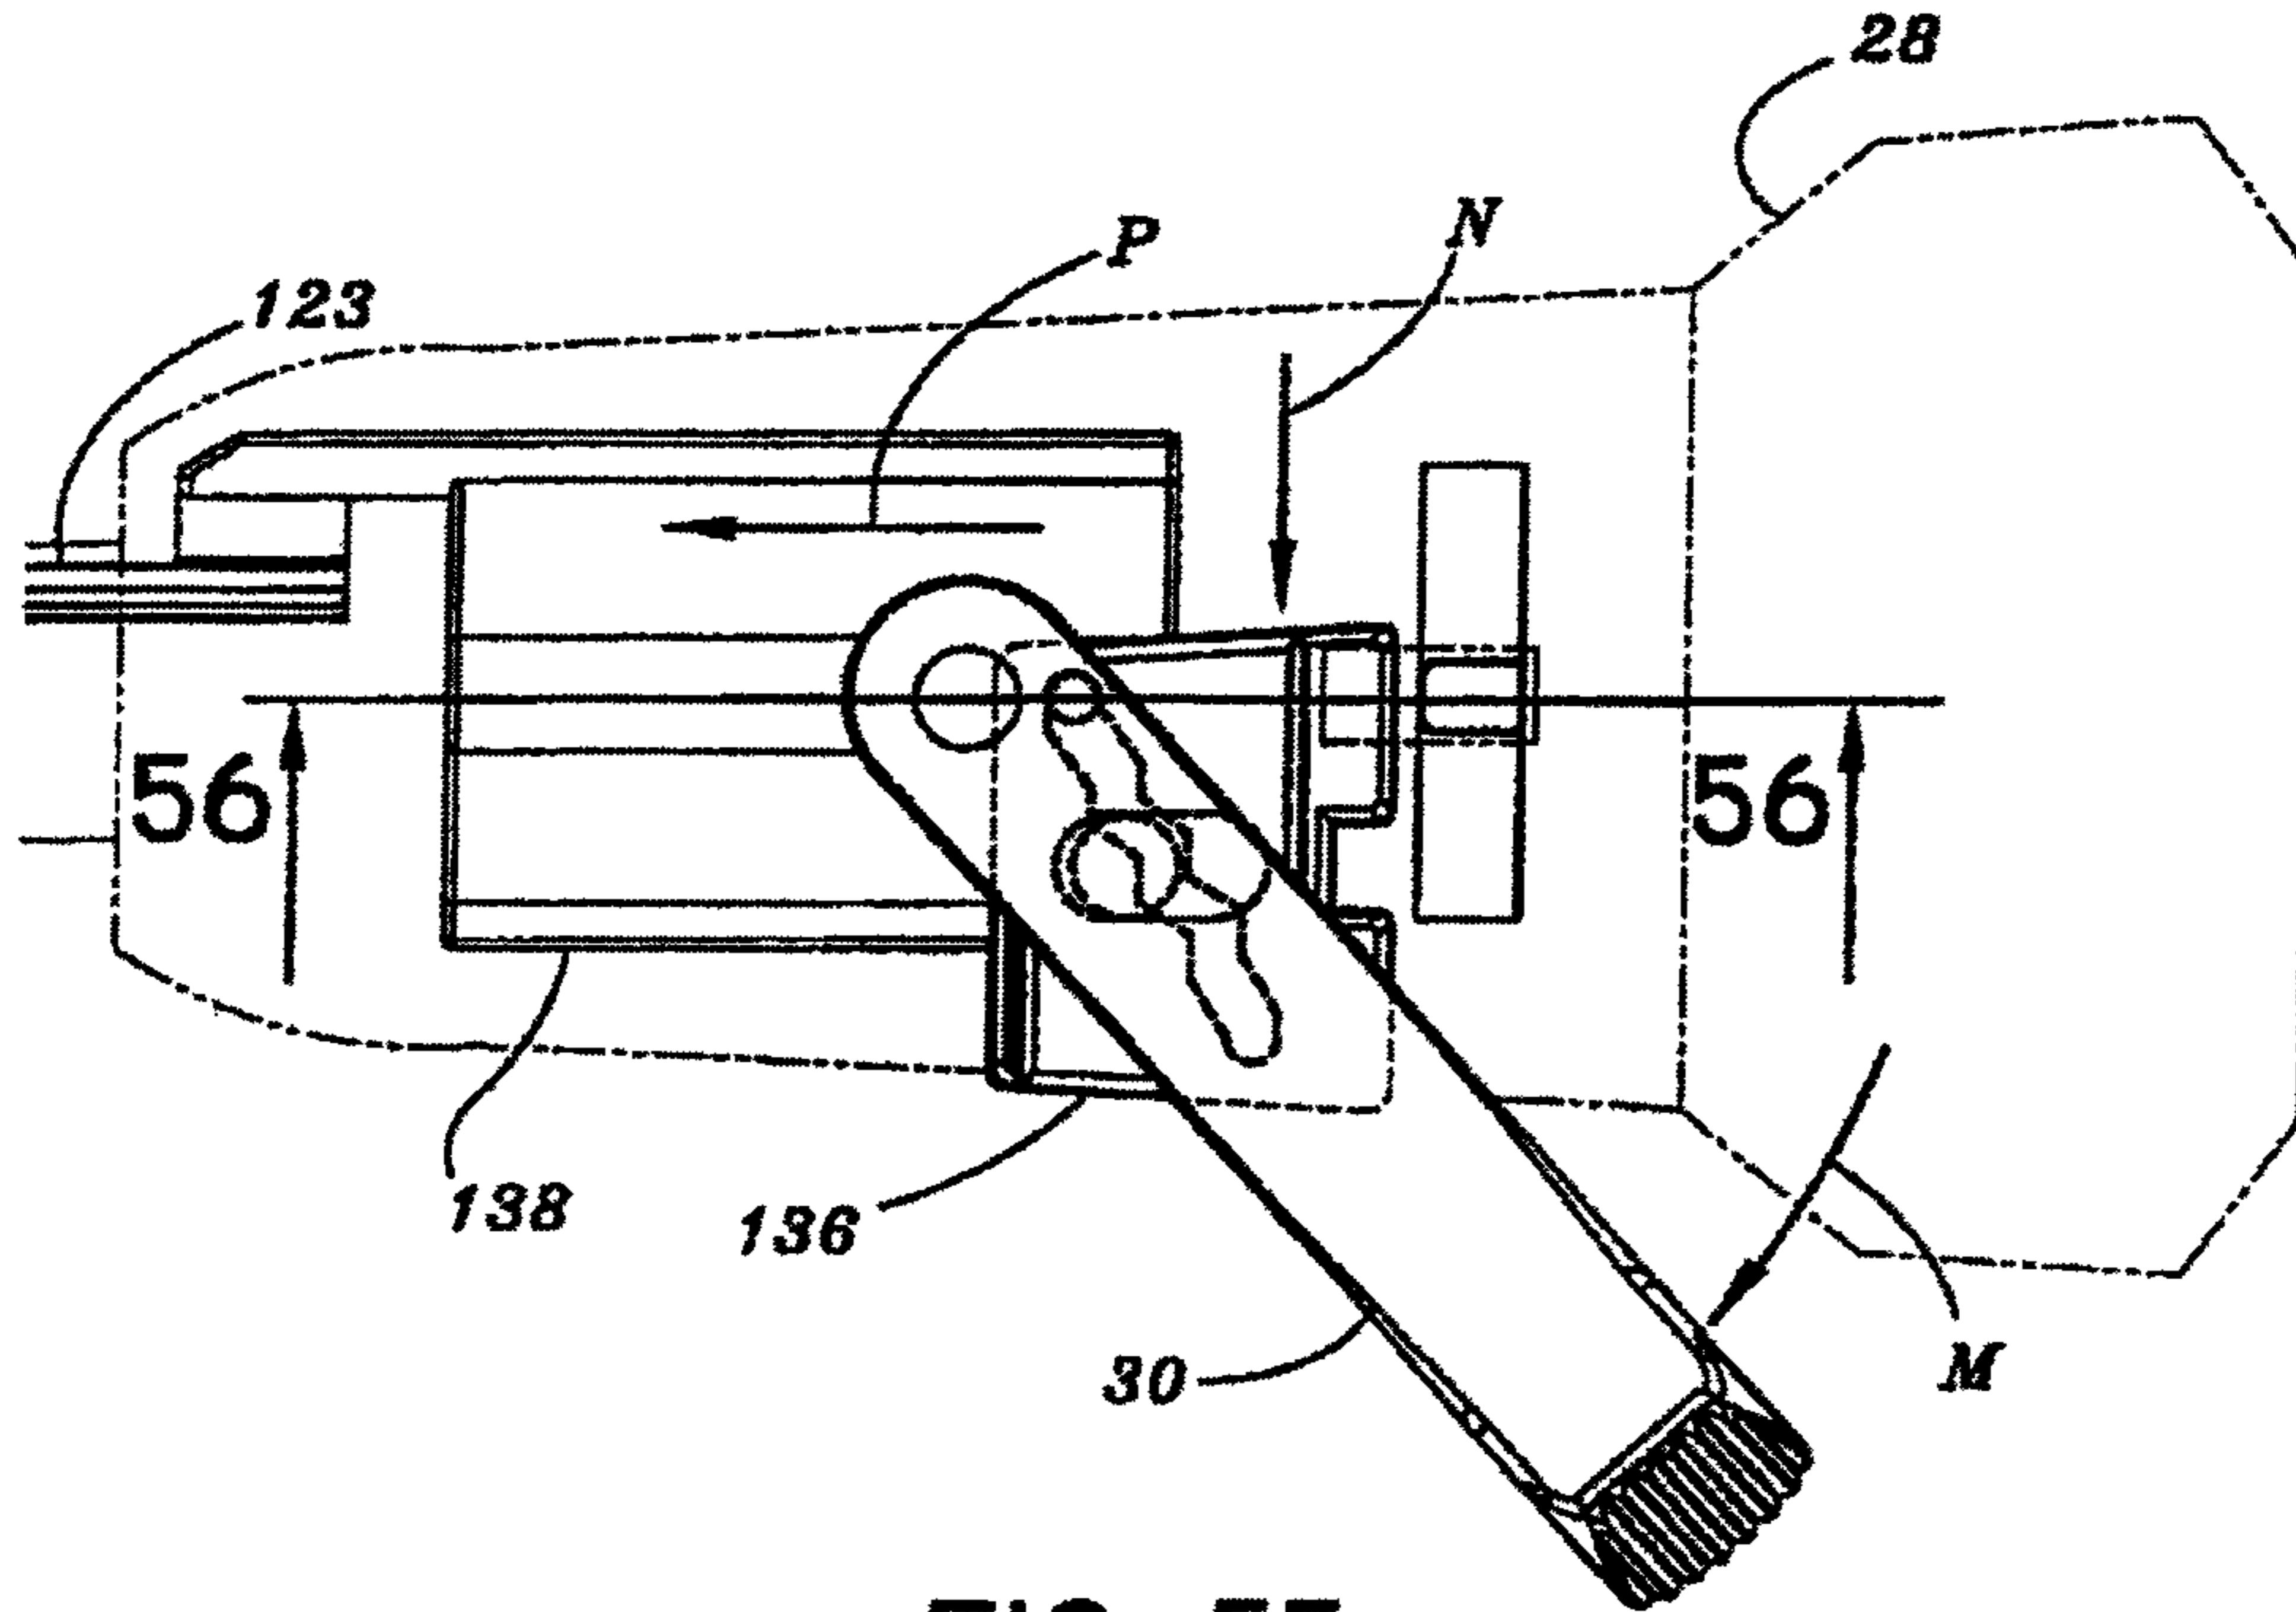


FIG. 55

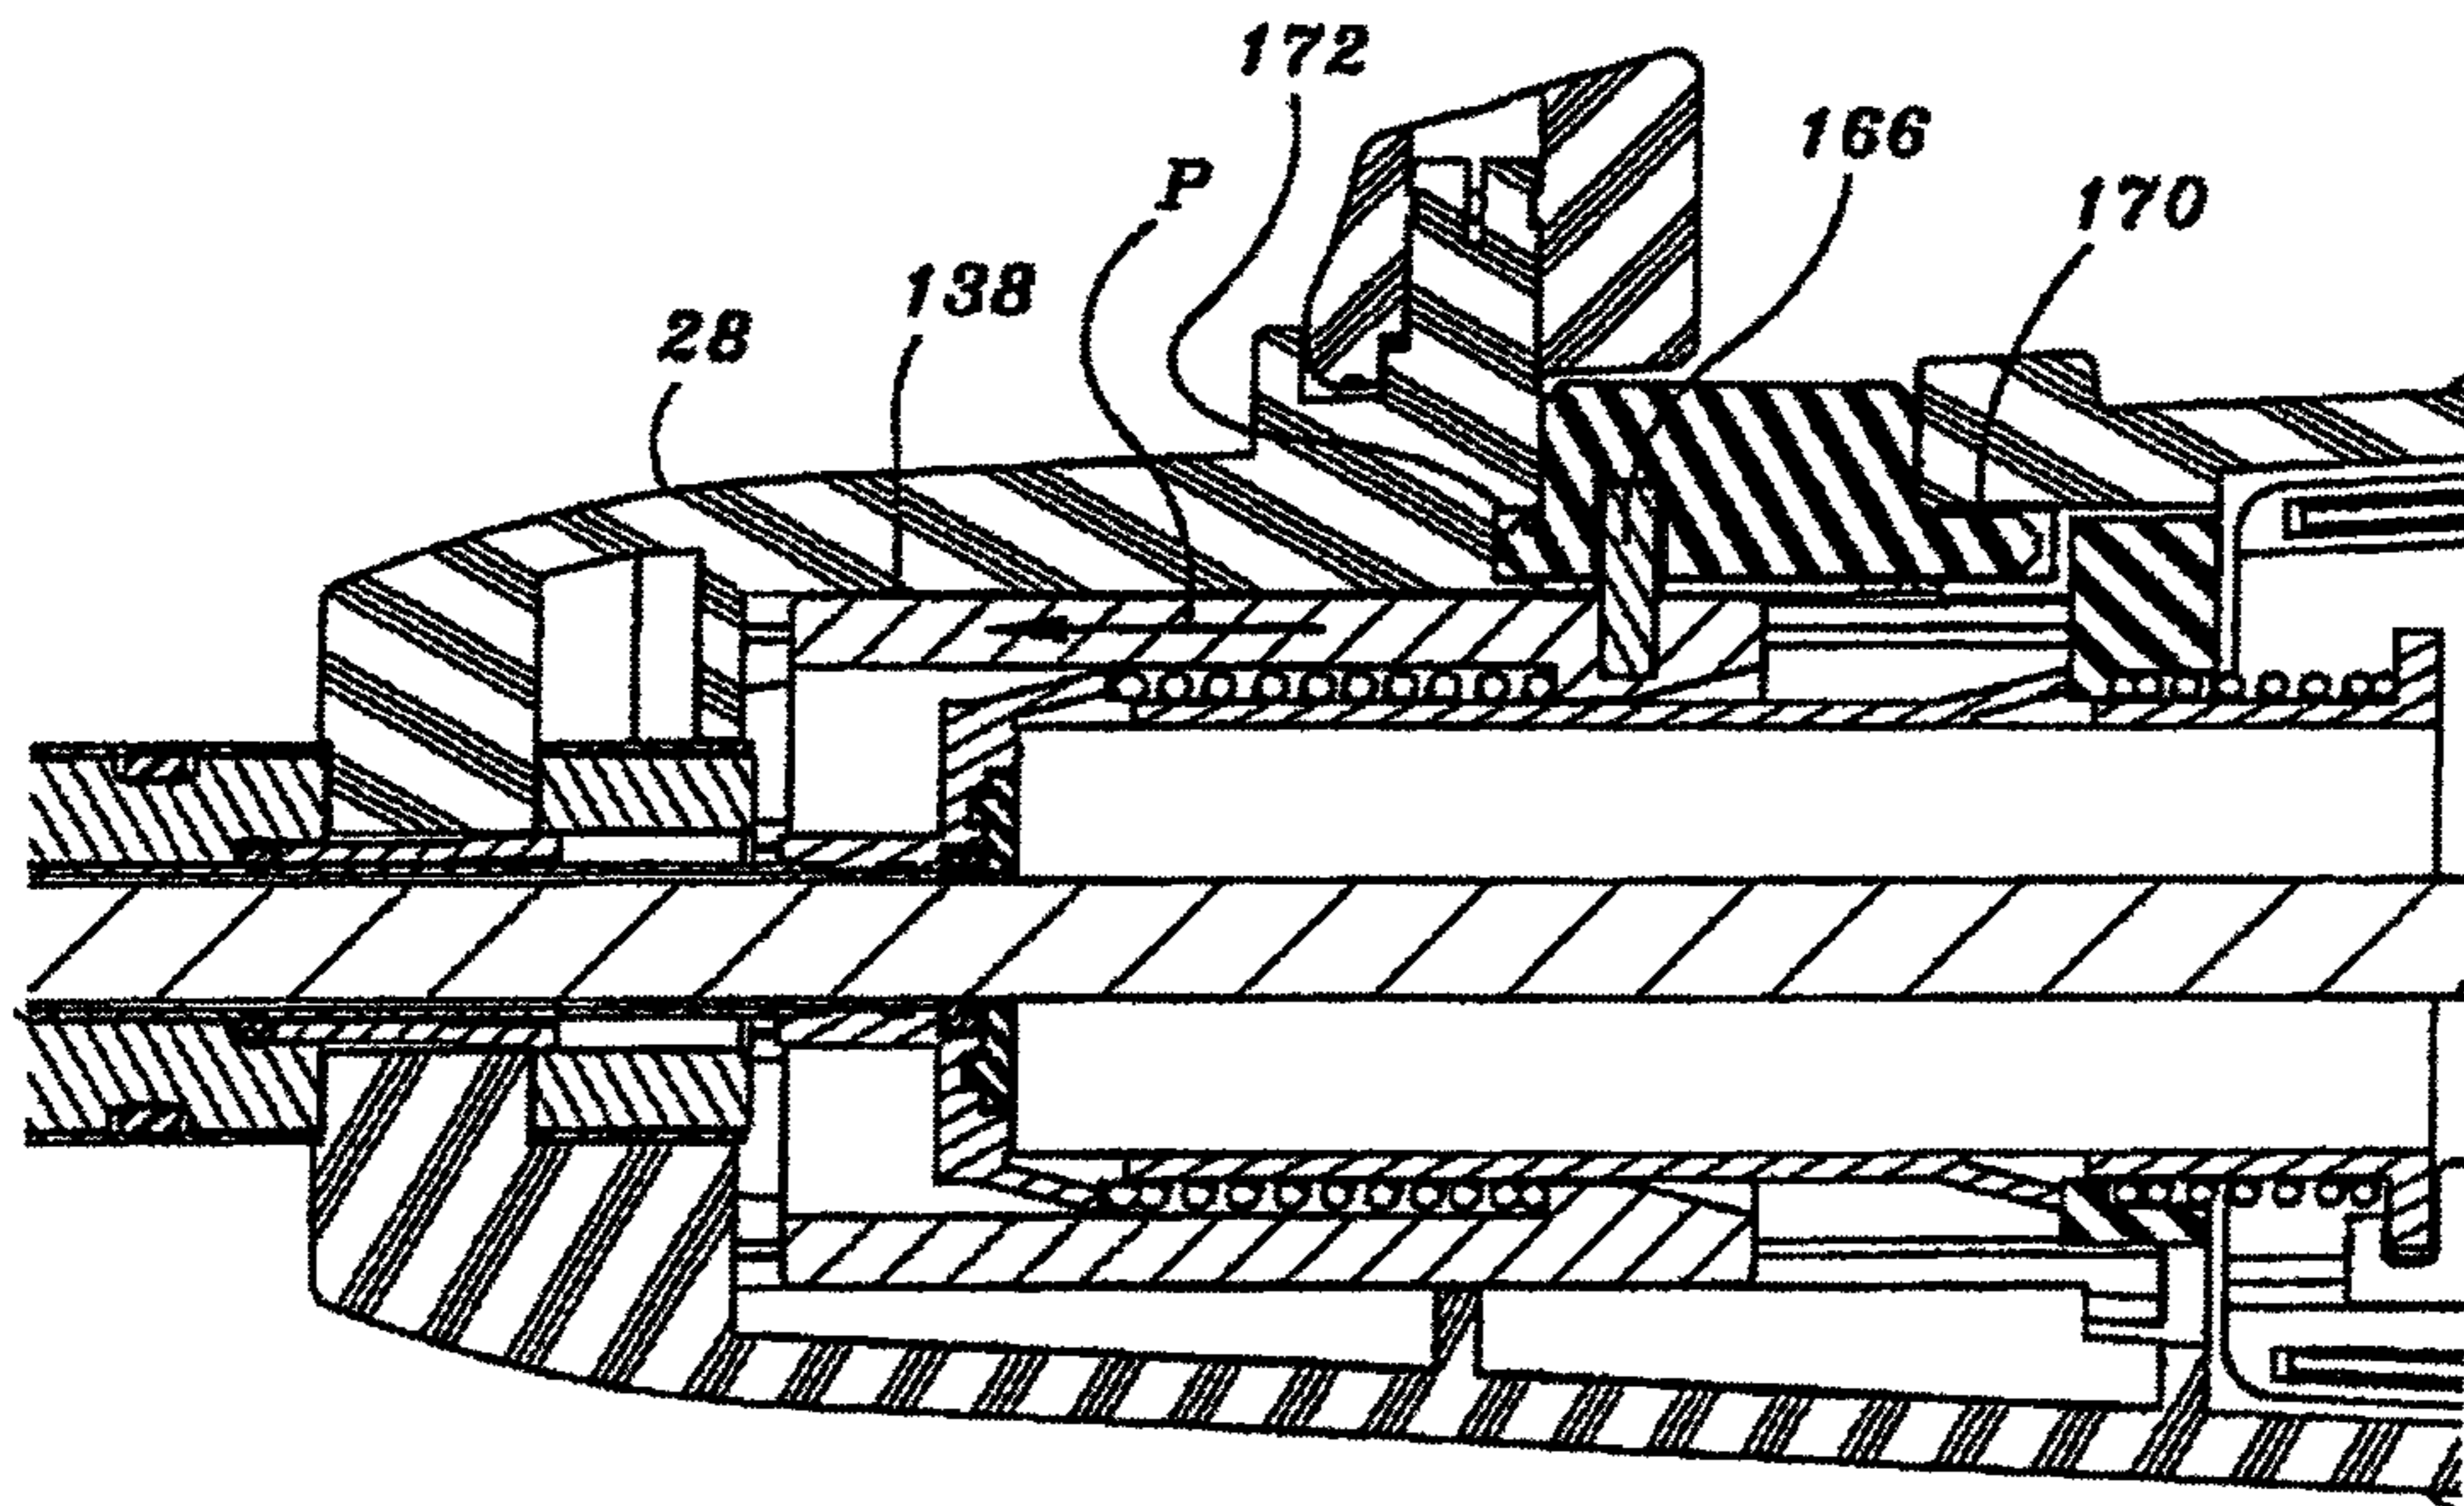


FIG. 56

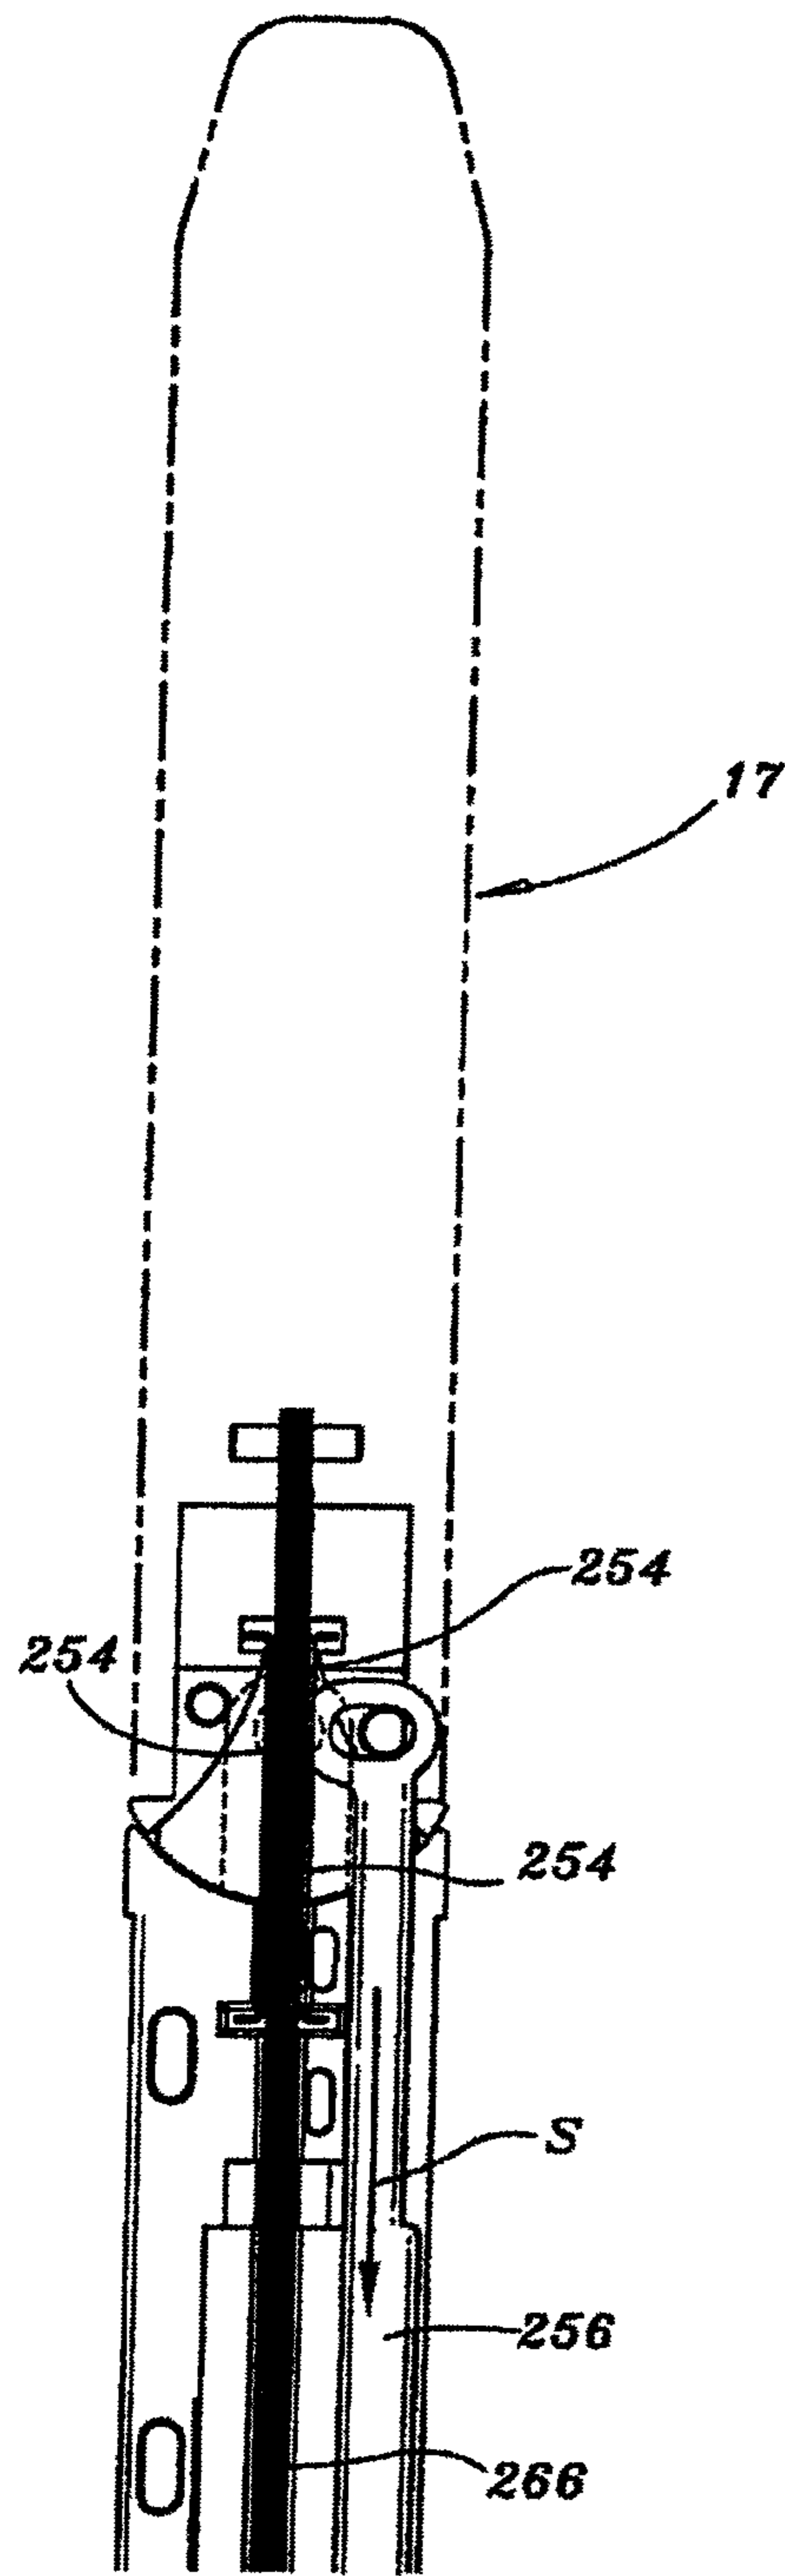


FIG. 60

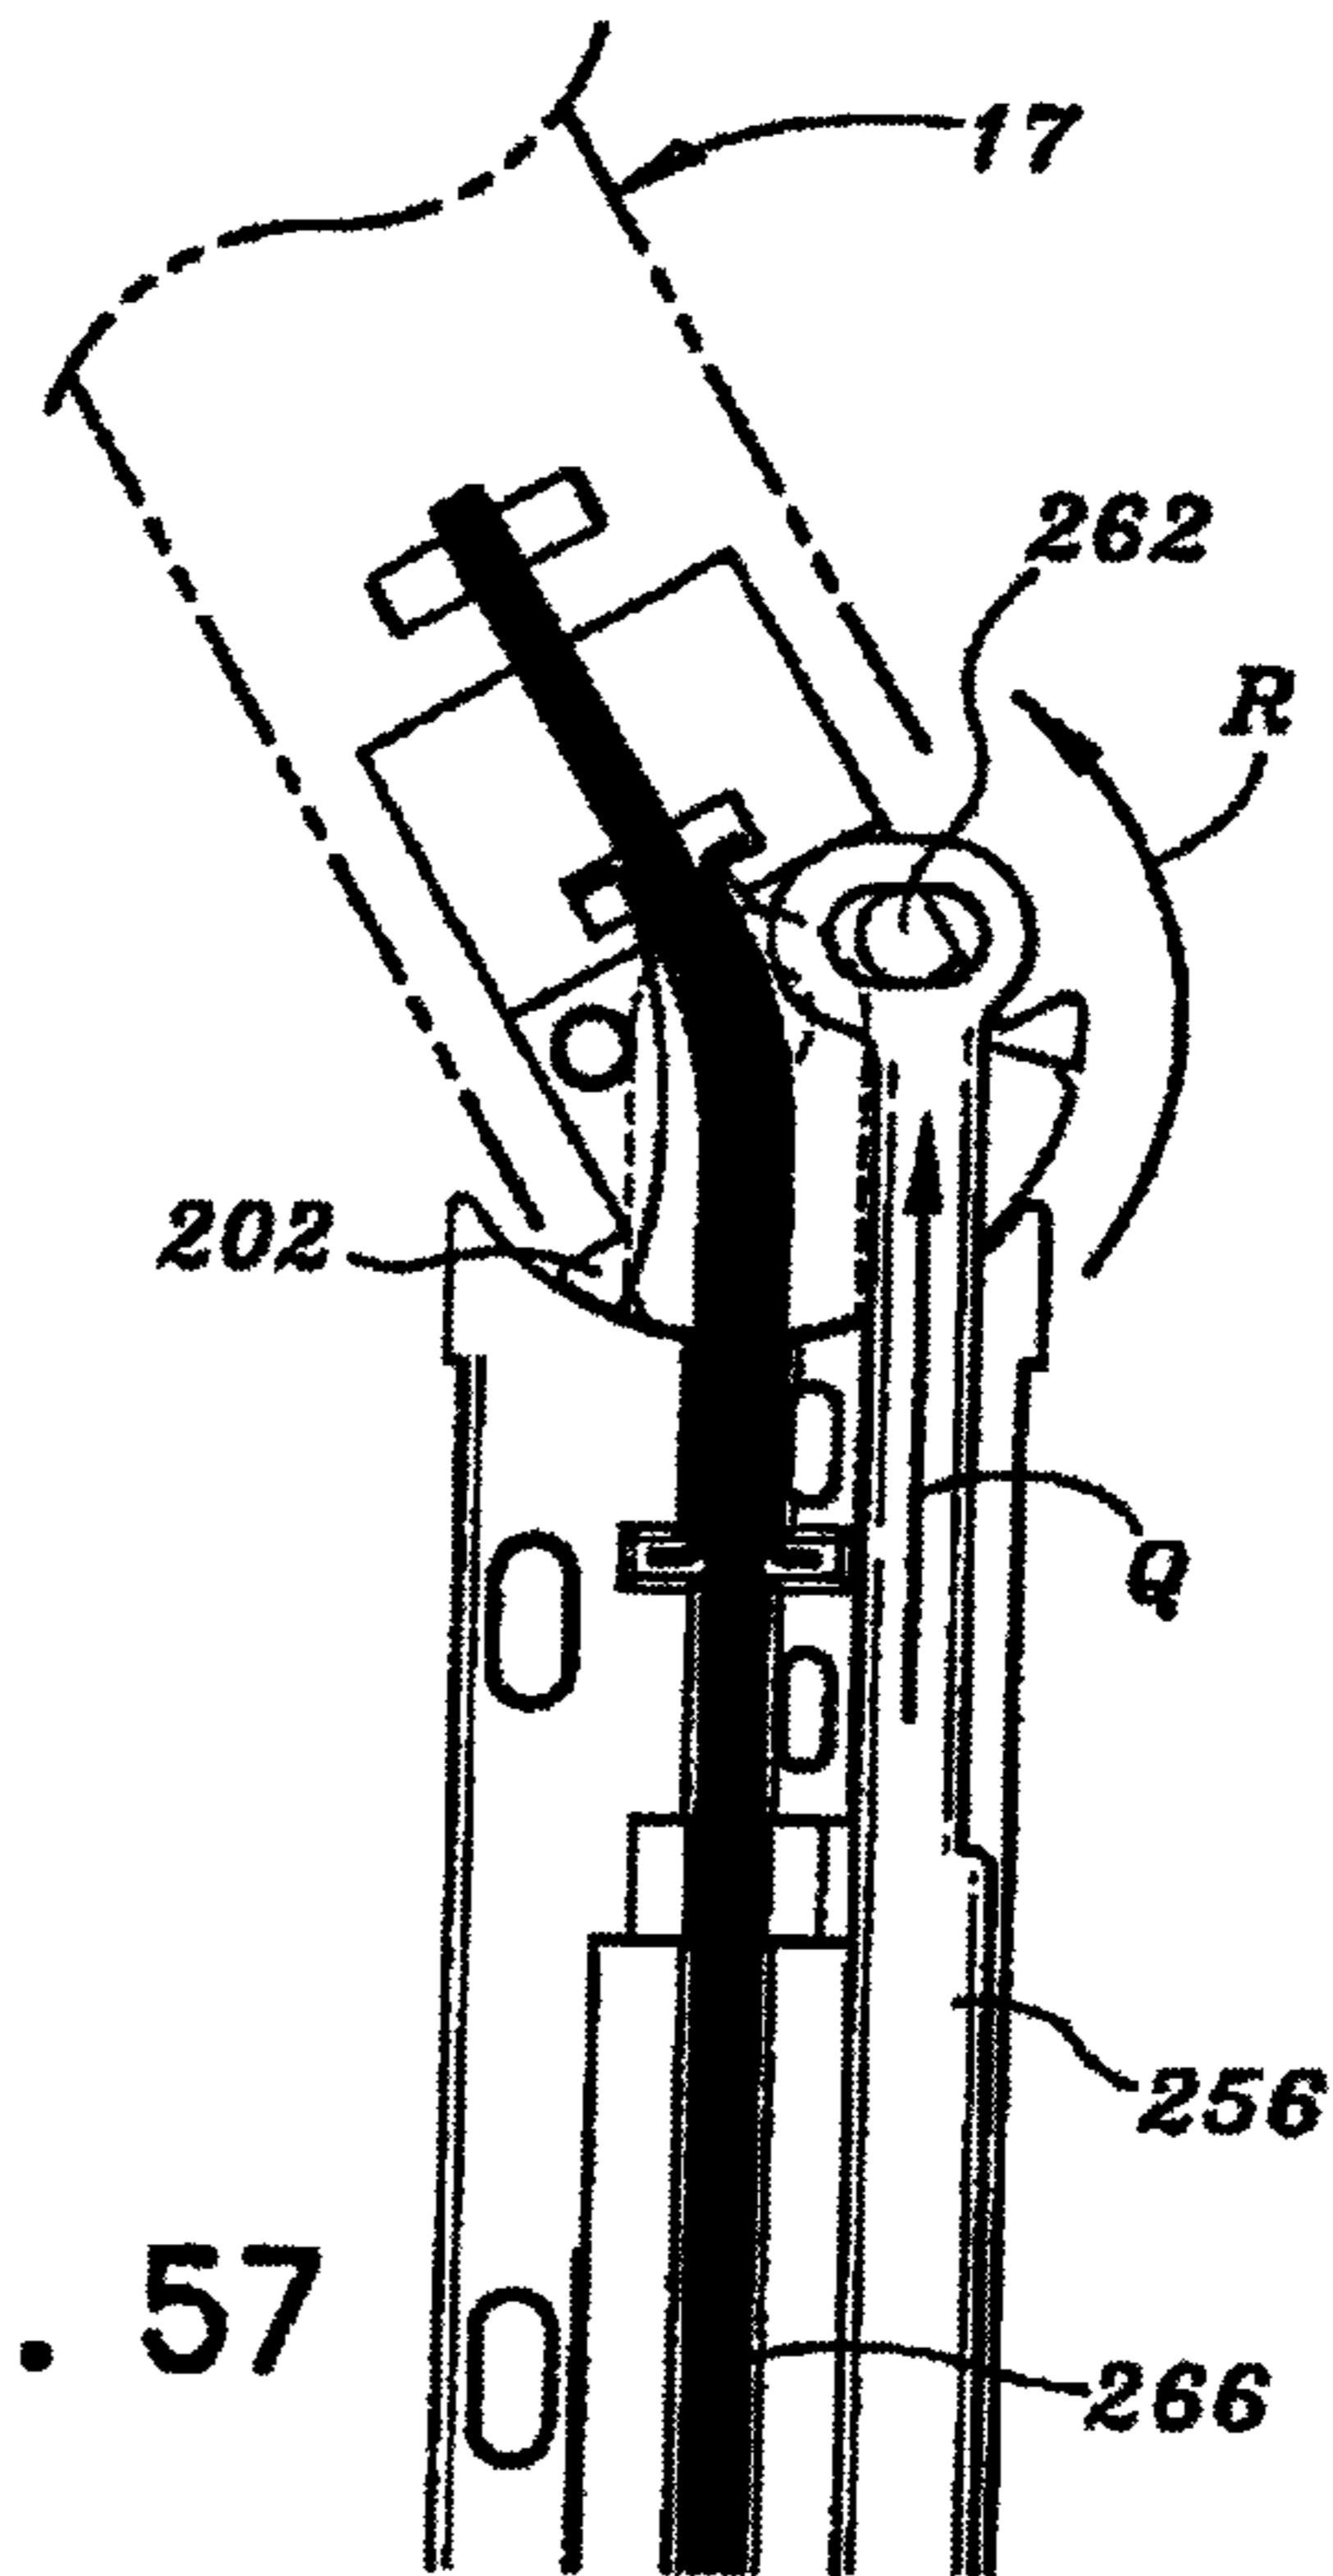


FIG. 57

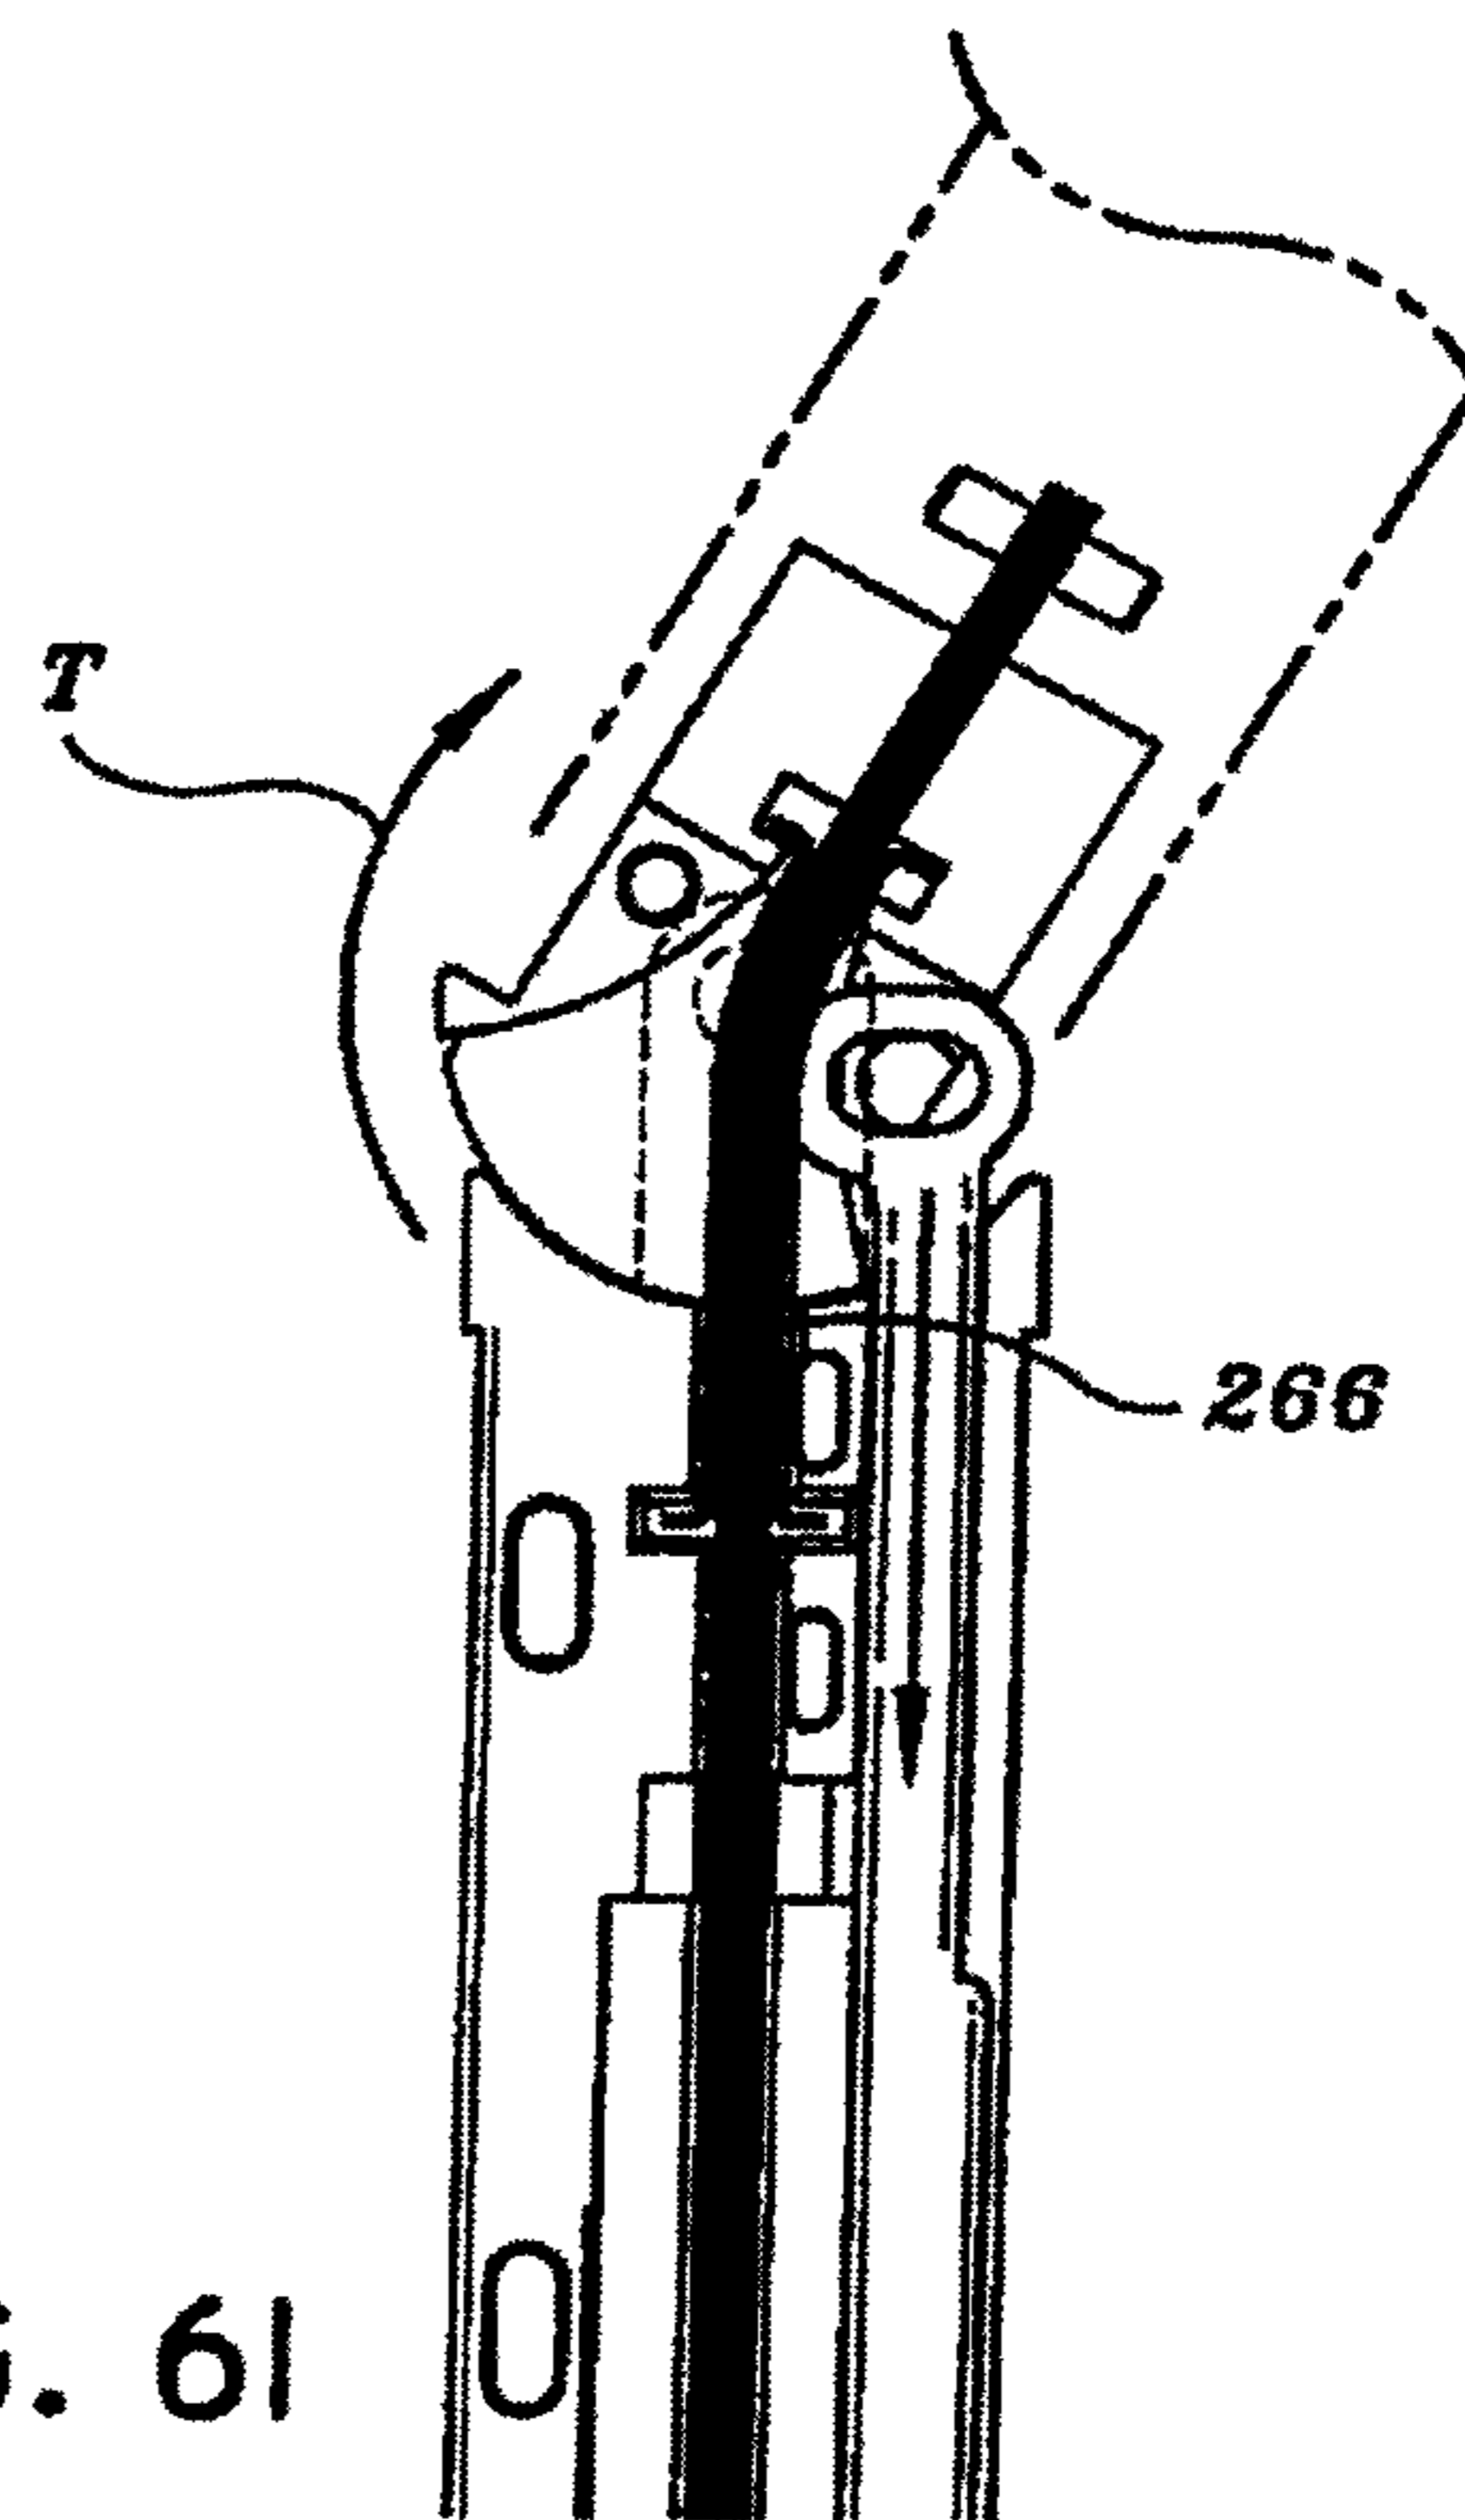


FIG. 61

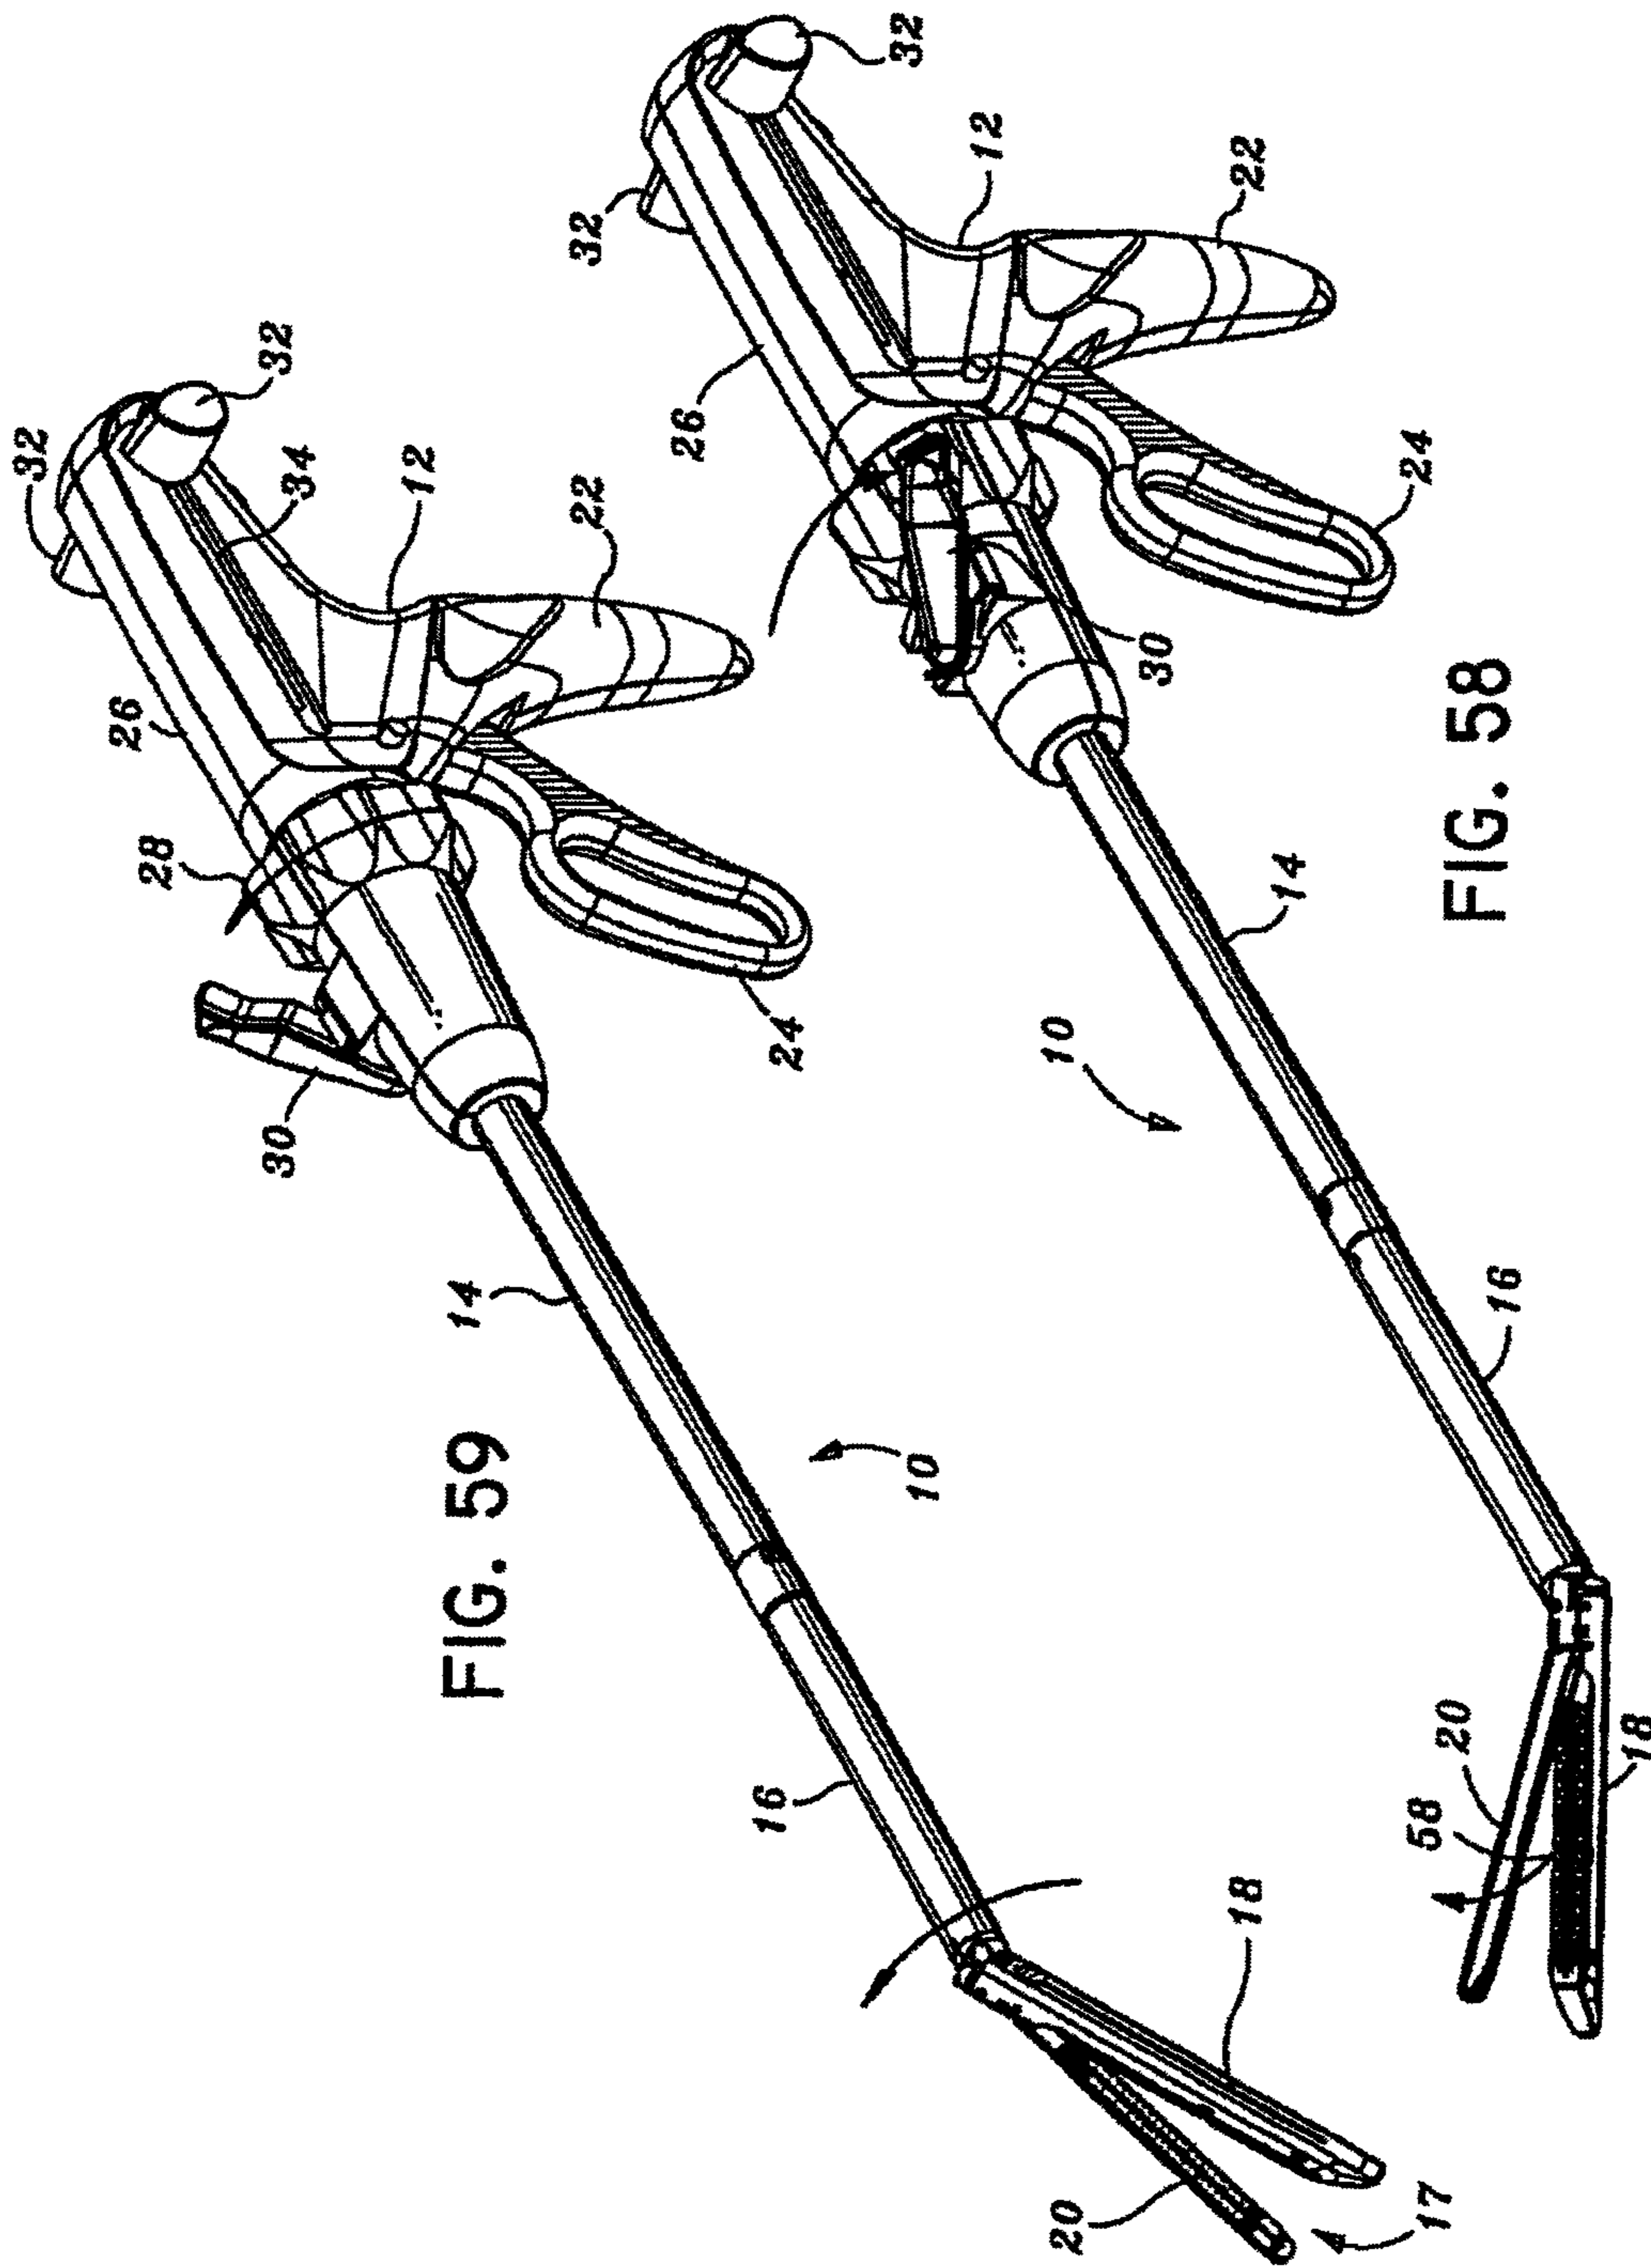


FIG. 59

FIG. 58

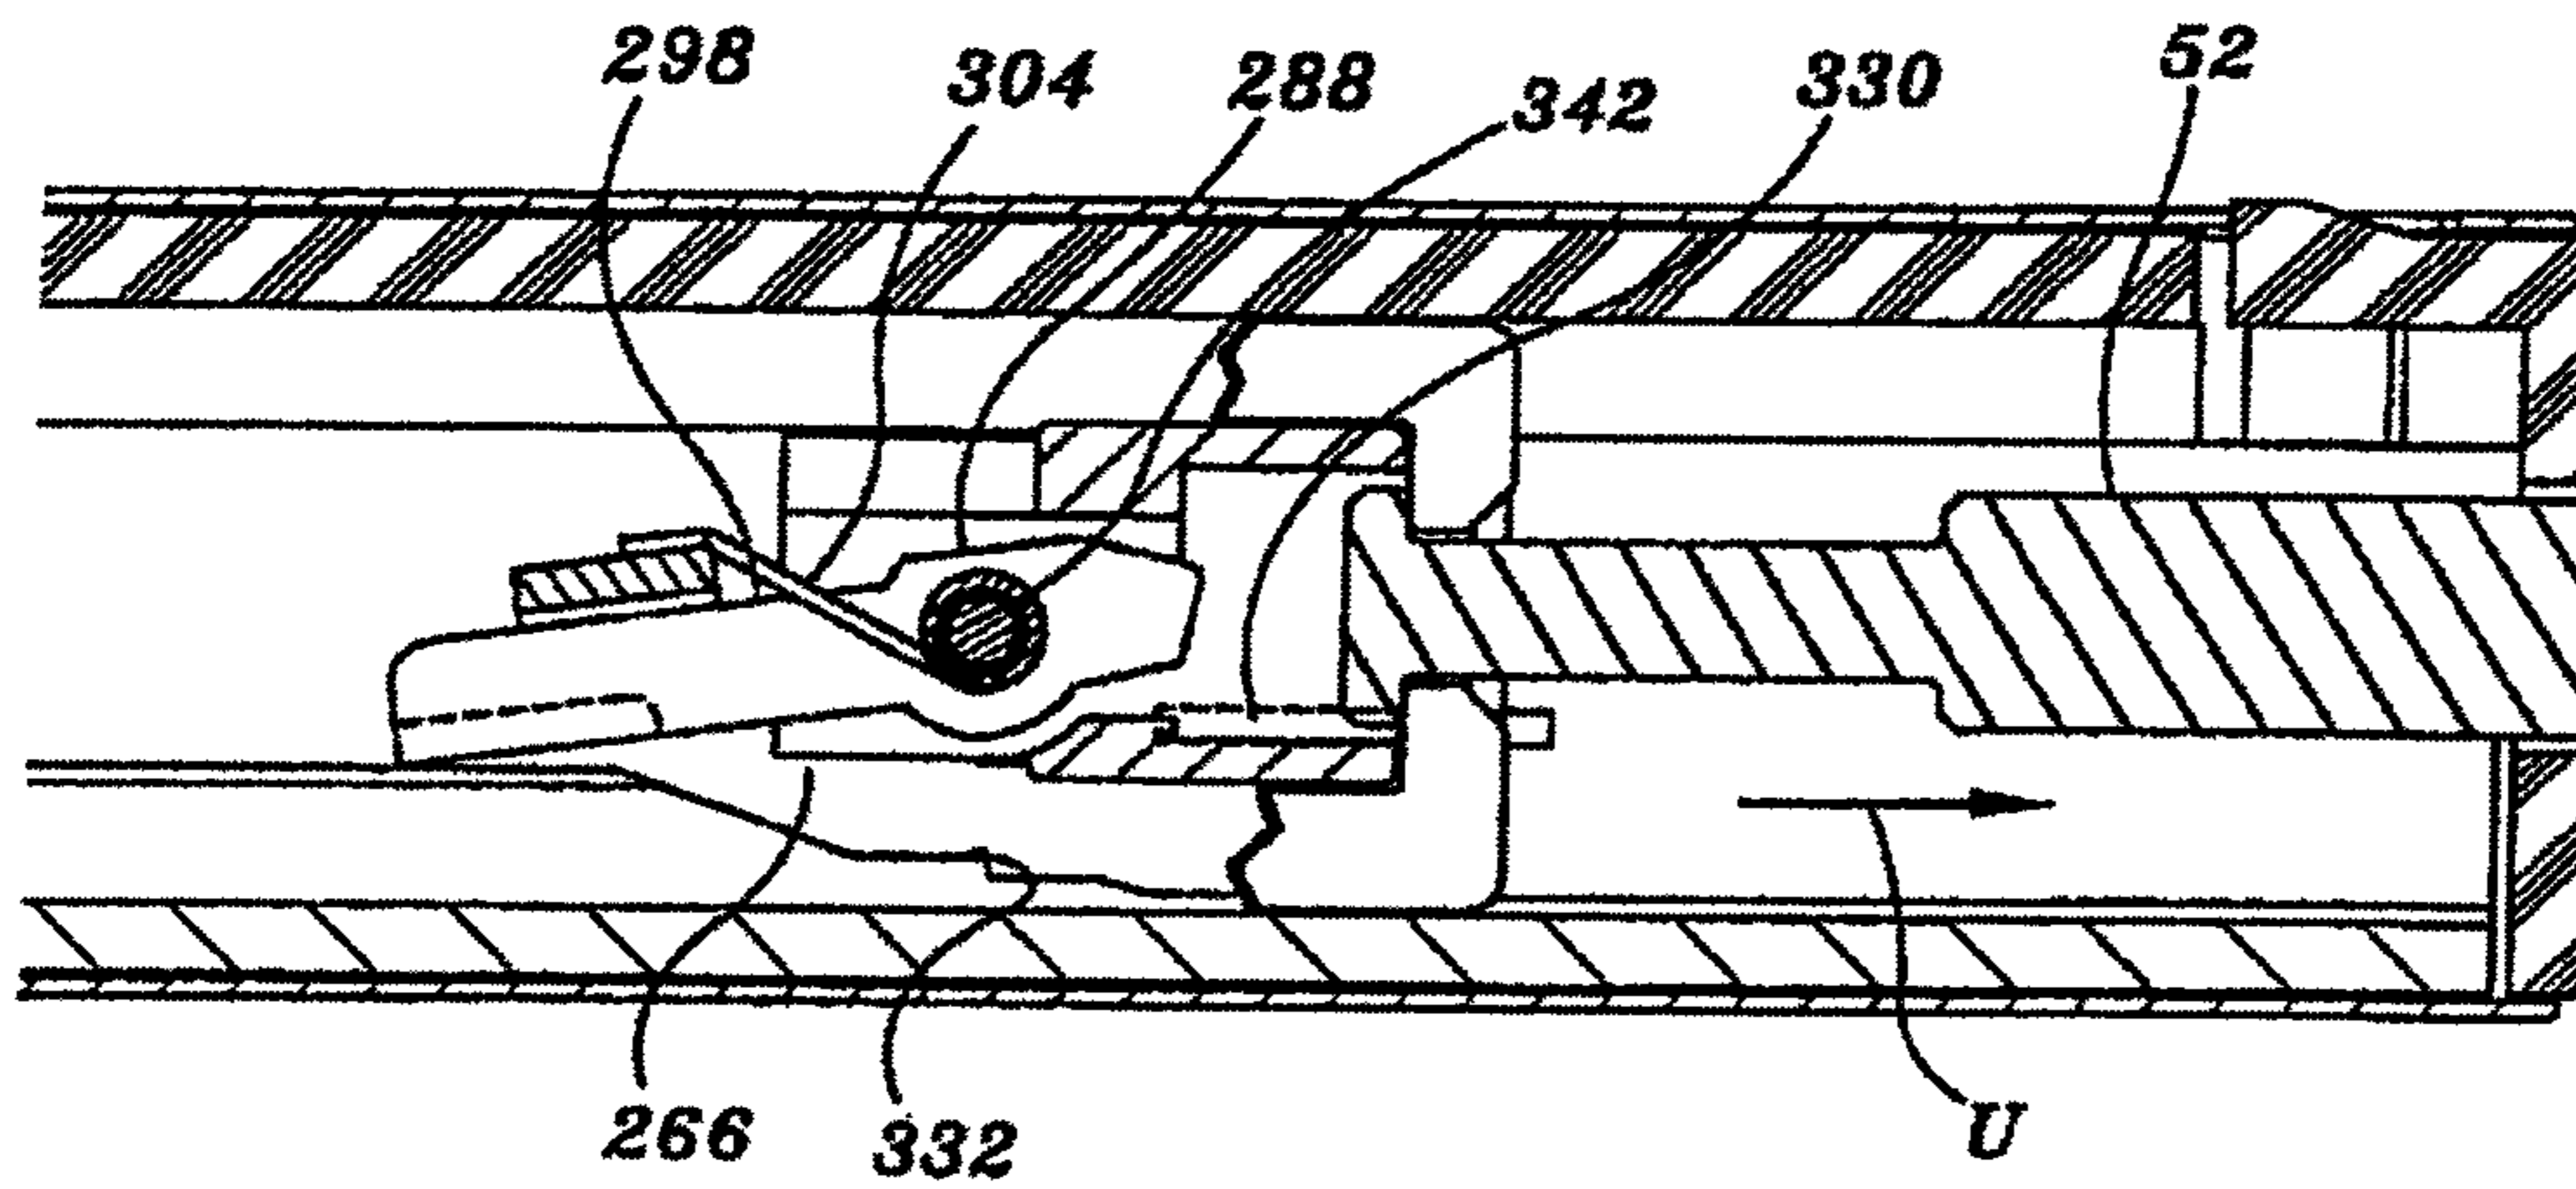


FIG. 62

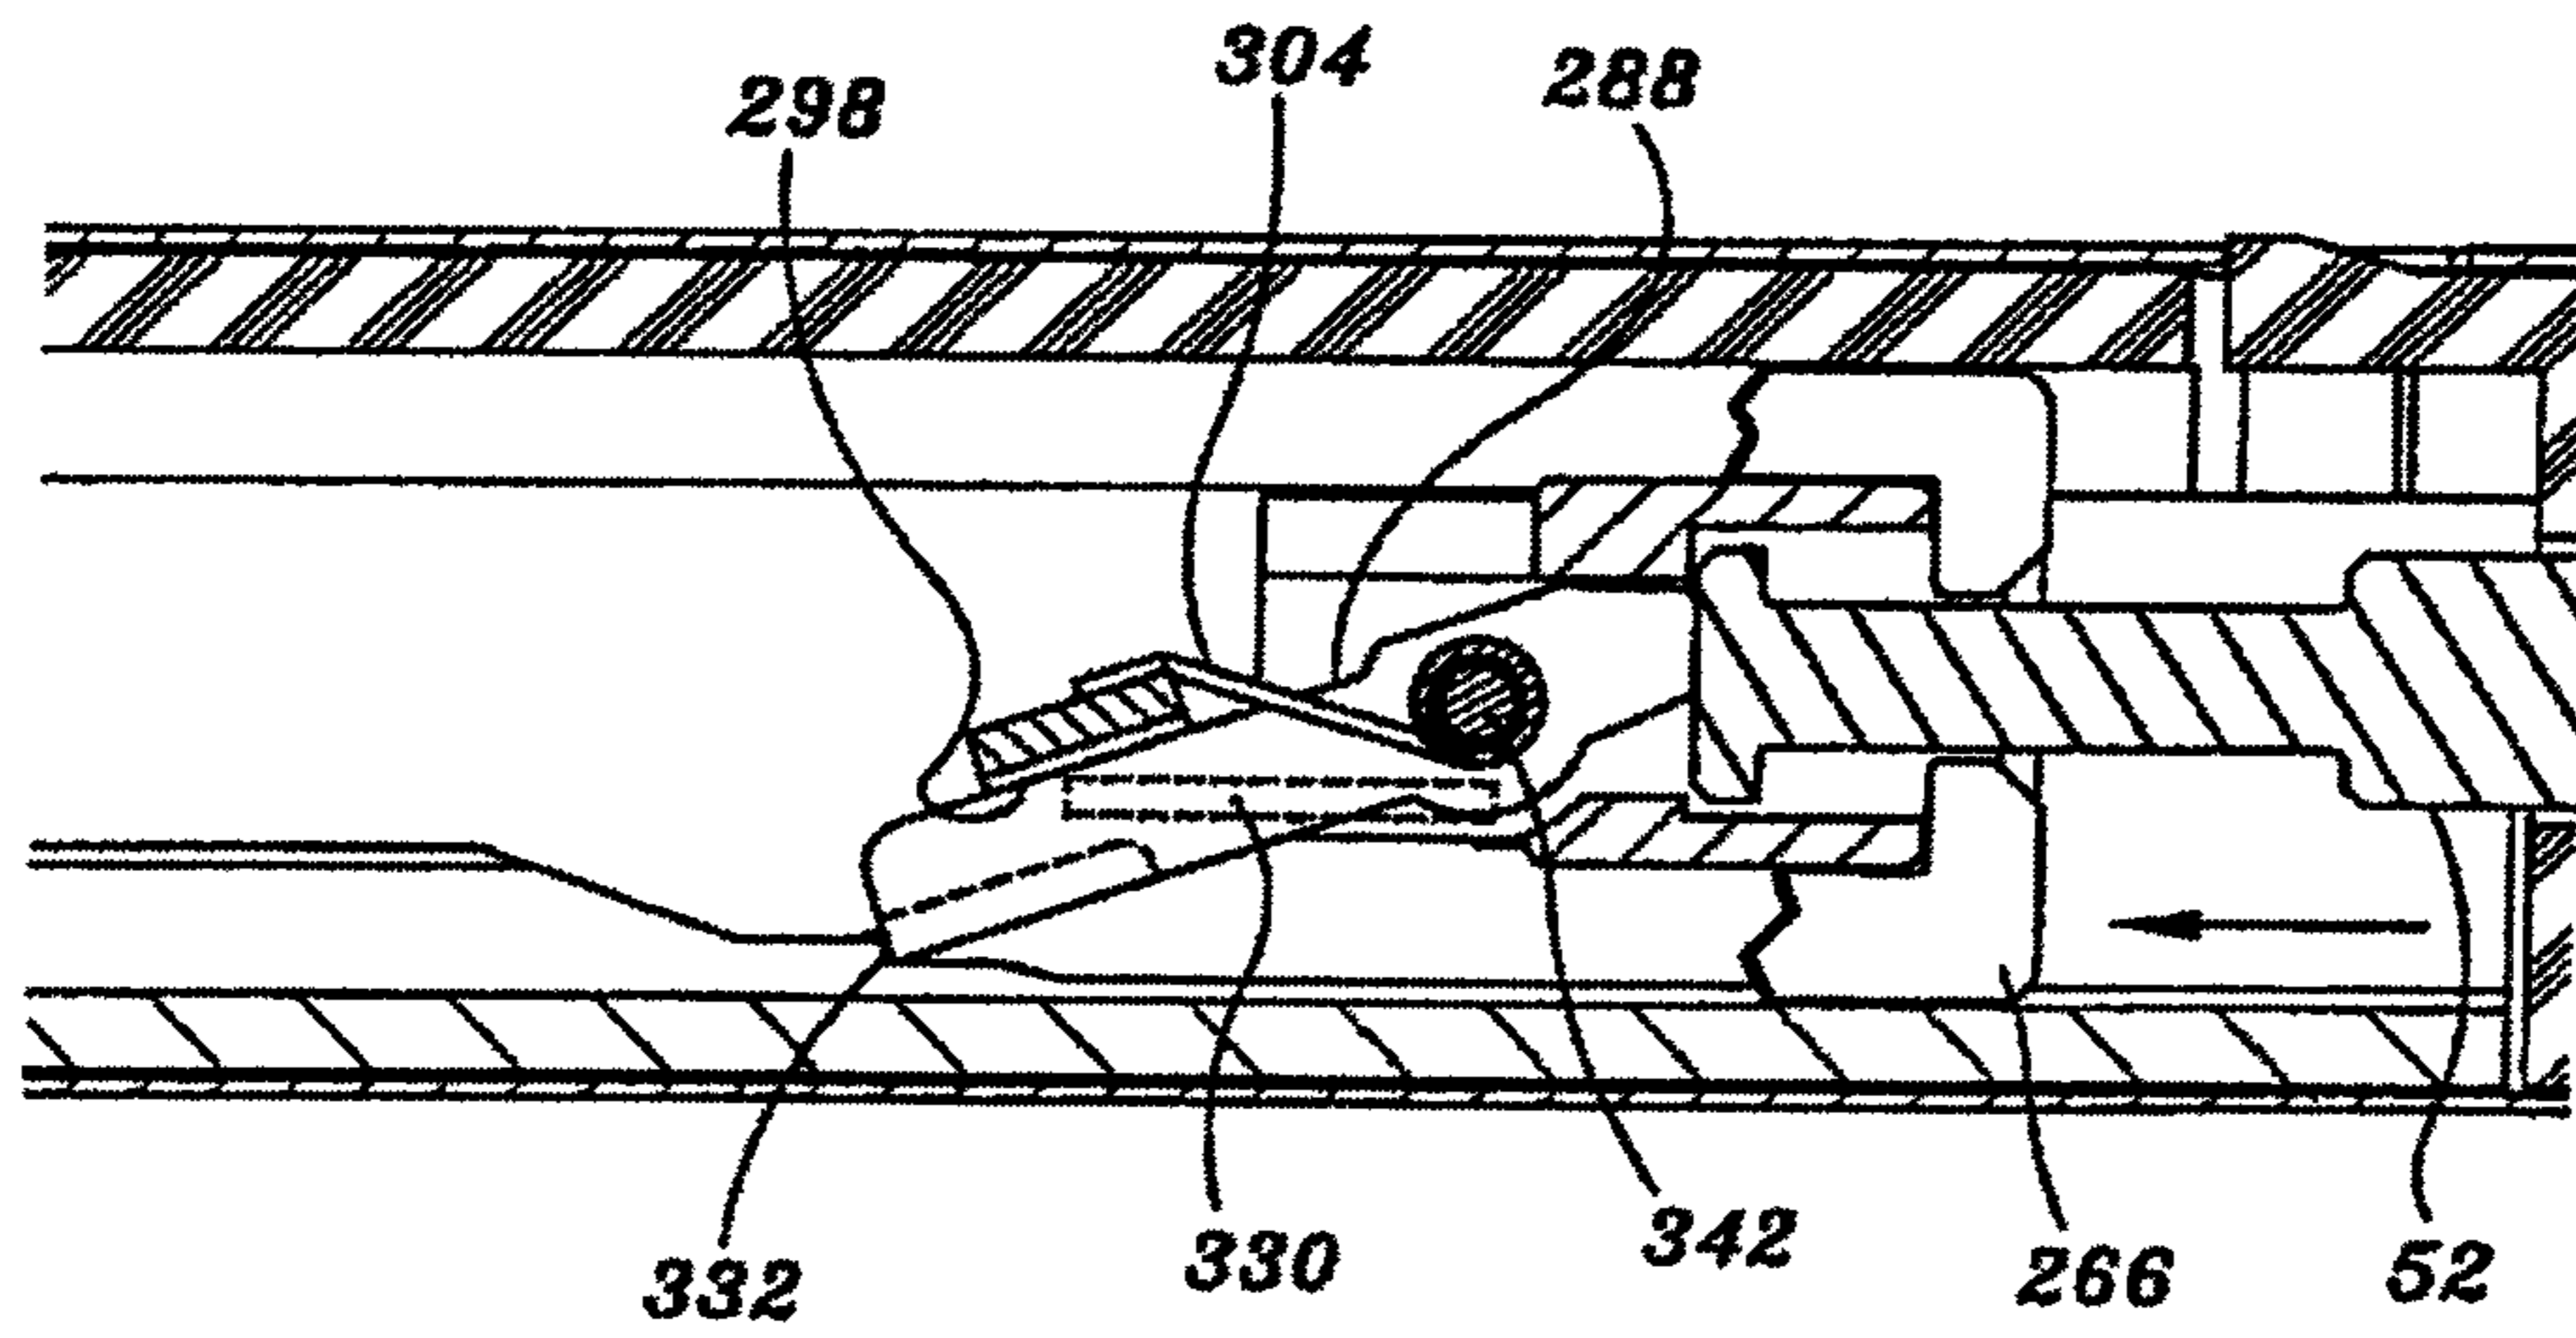


FIG. 63

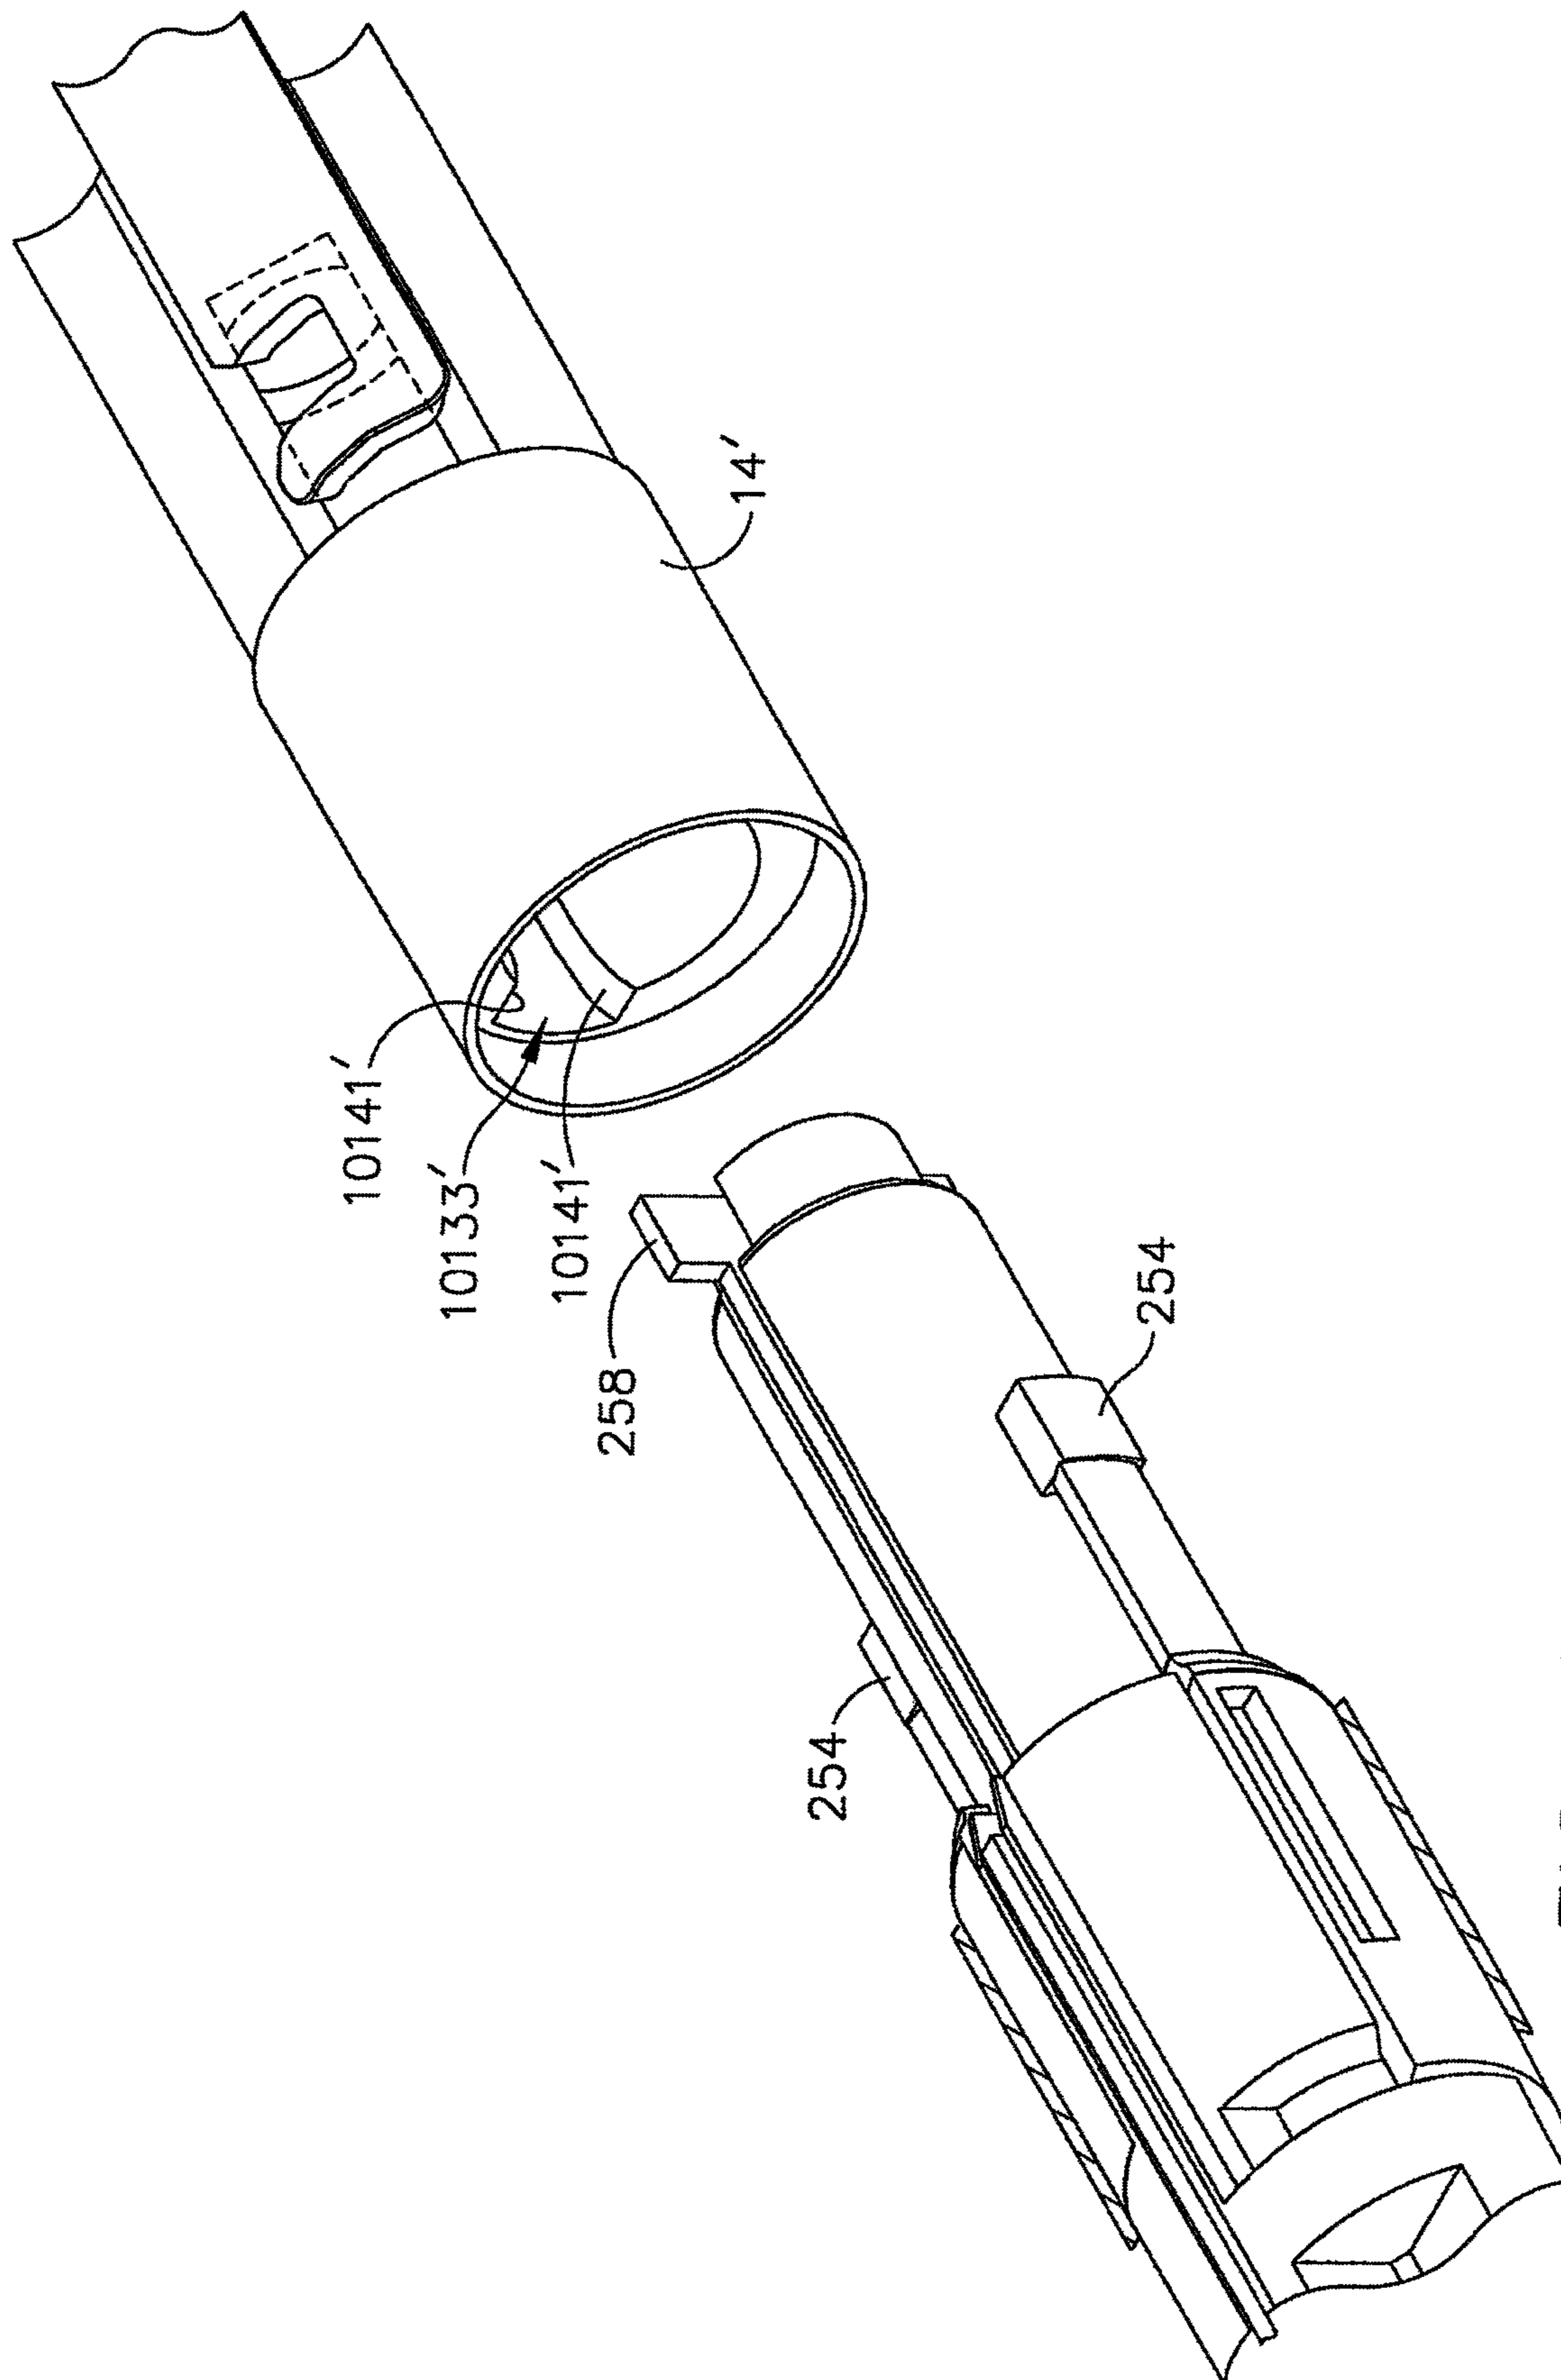


FIG. 64



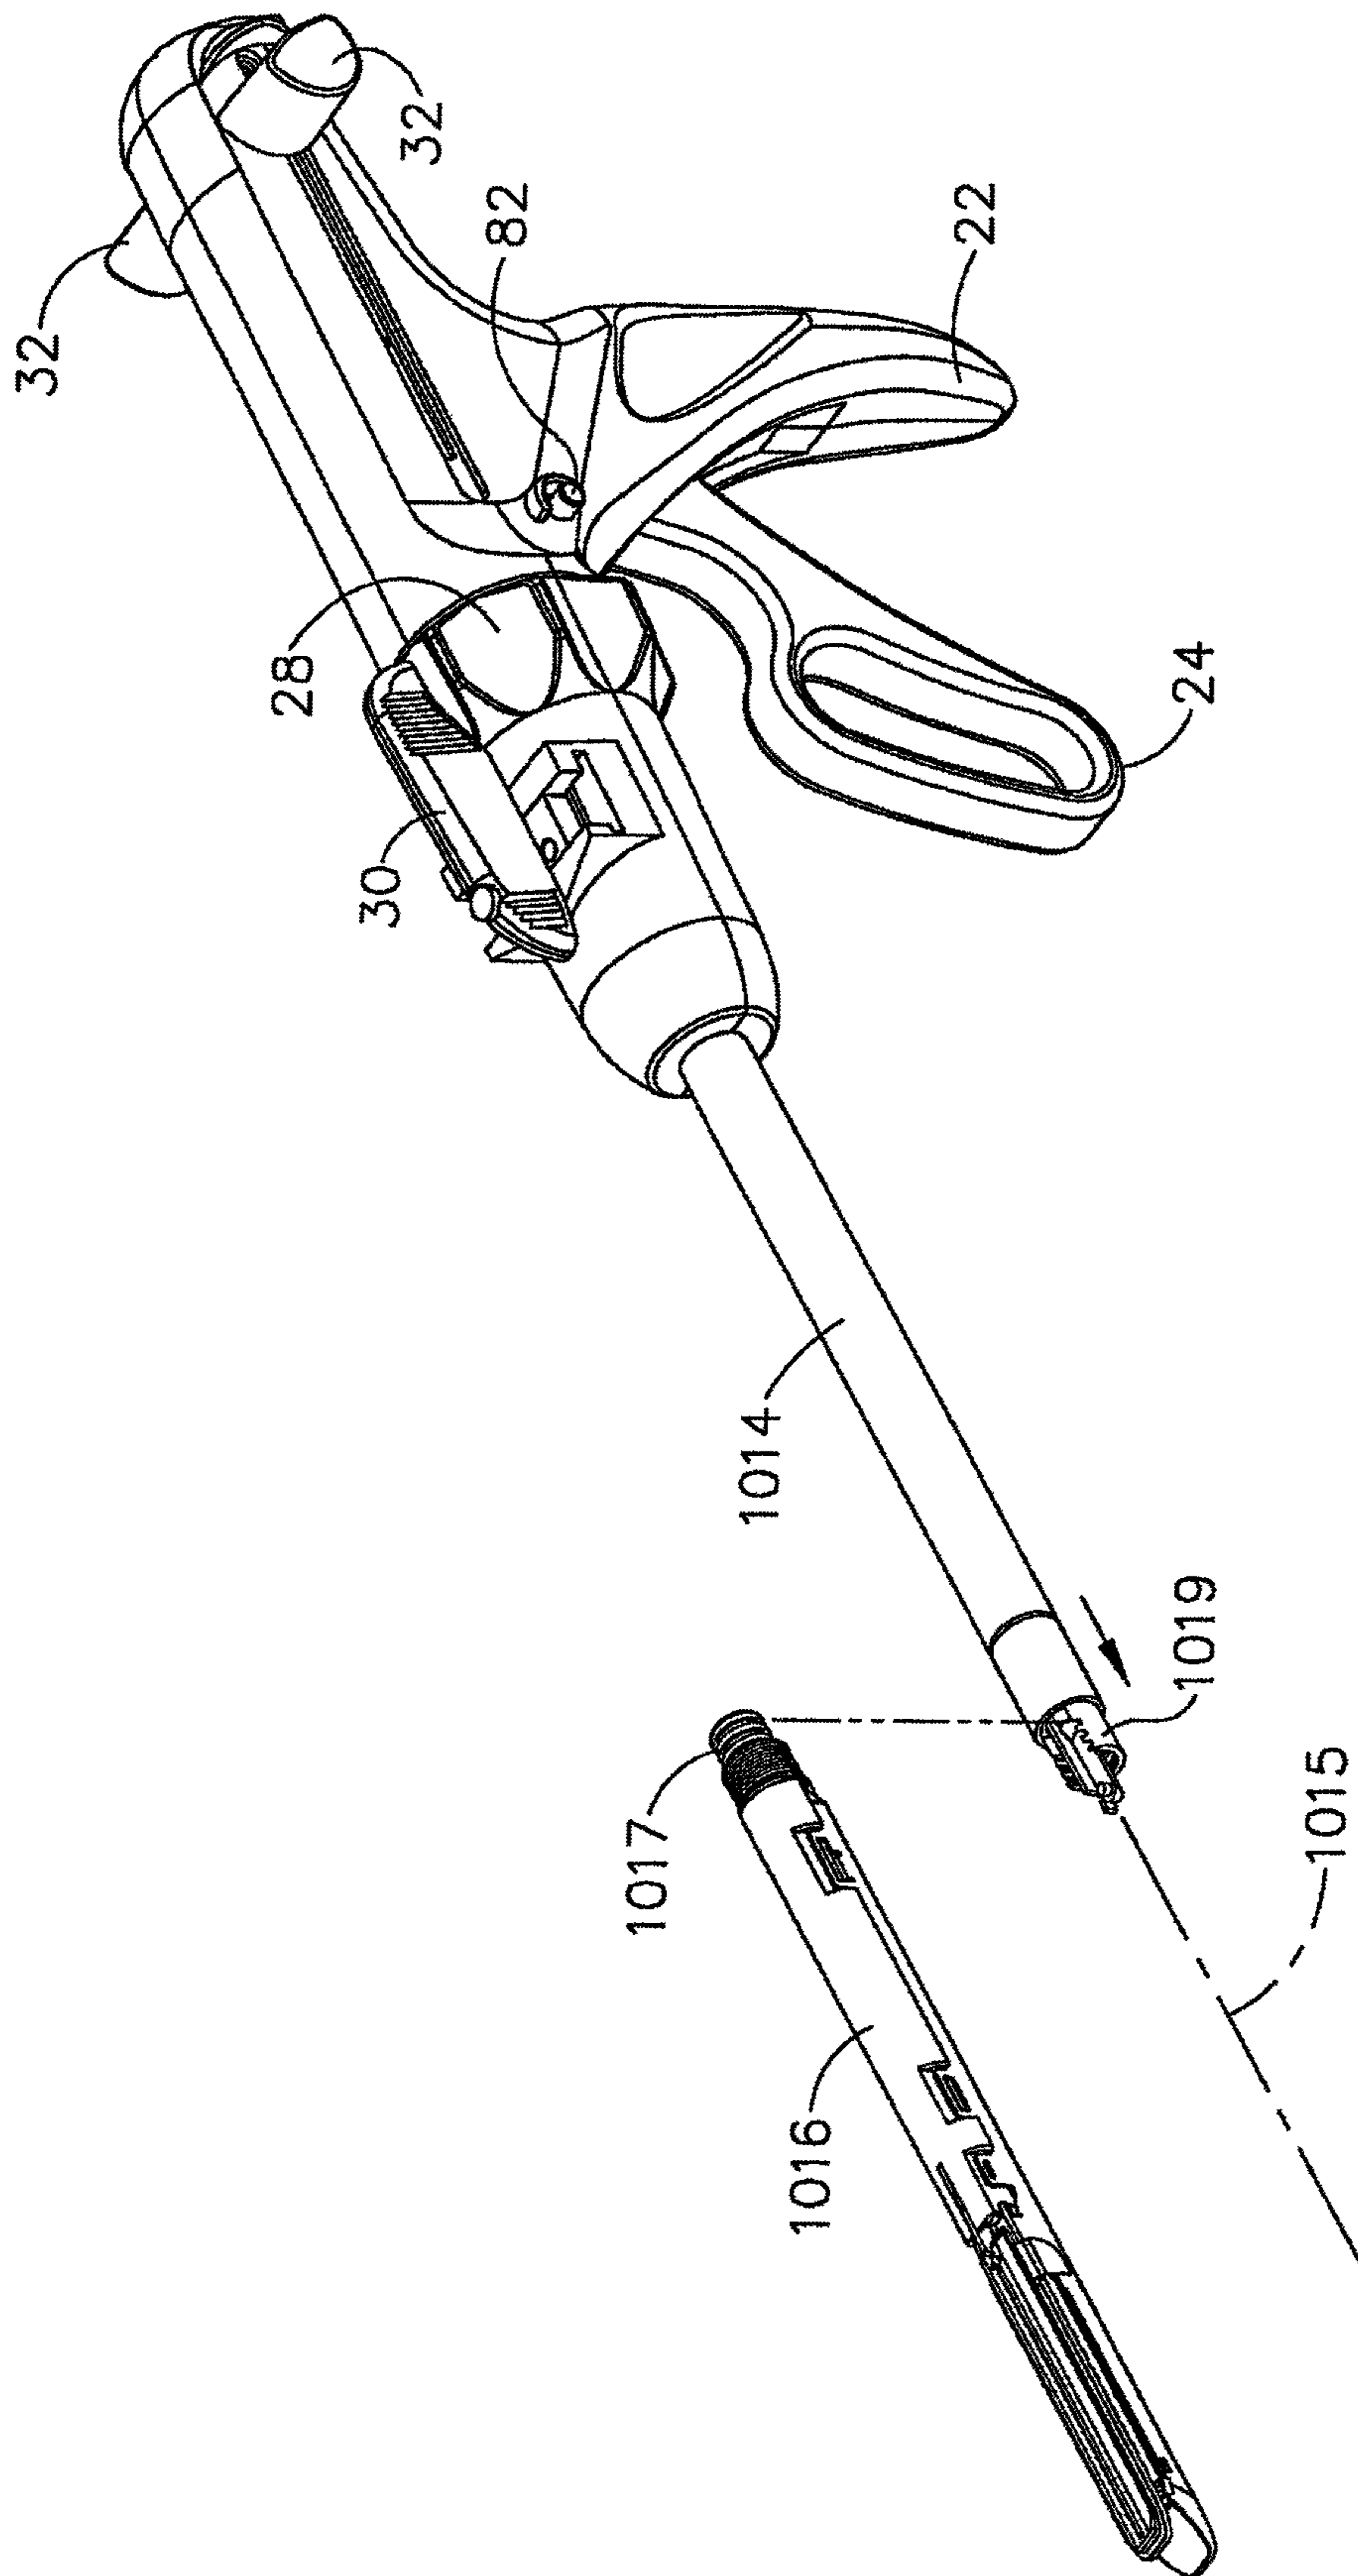


FIG. 65

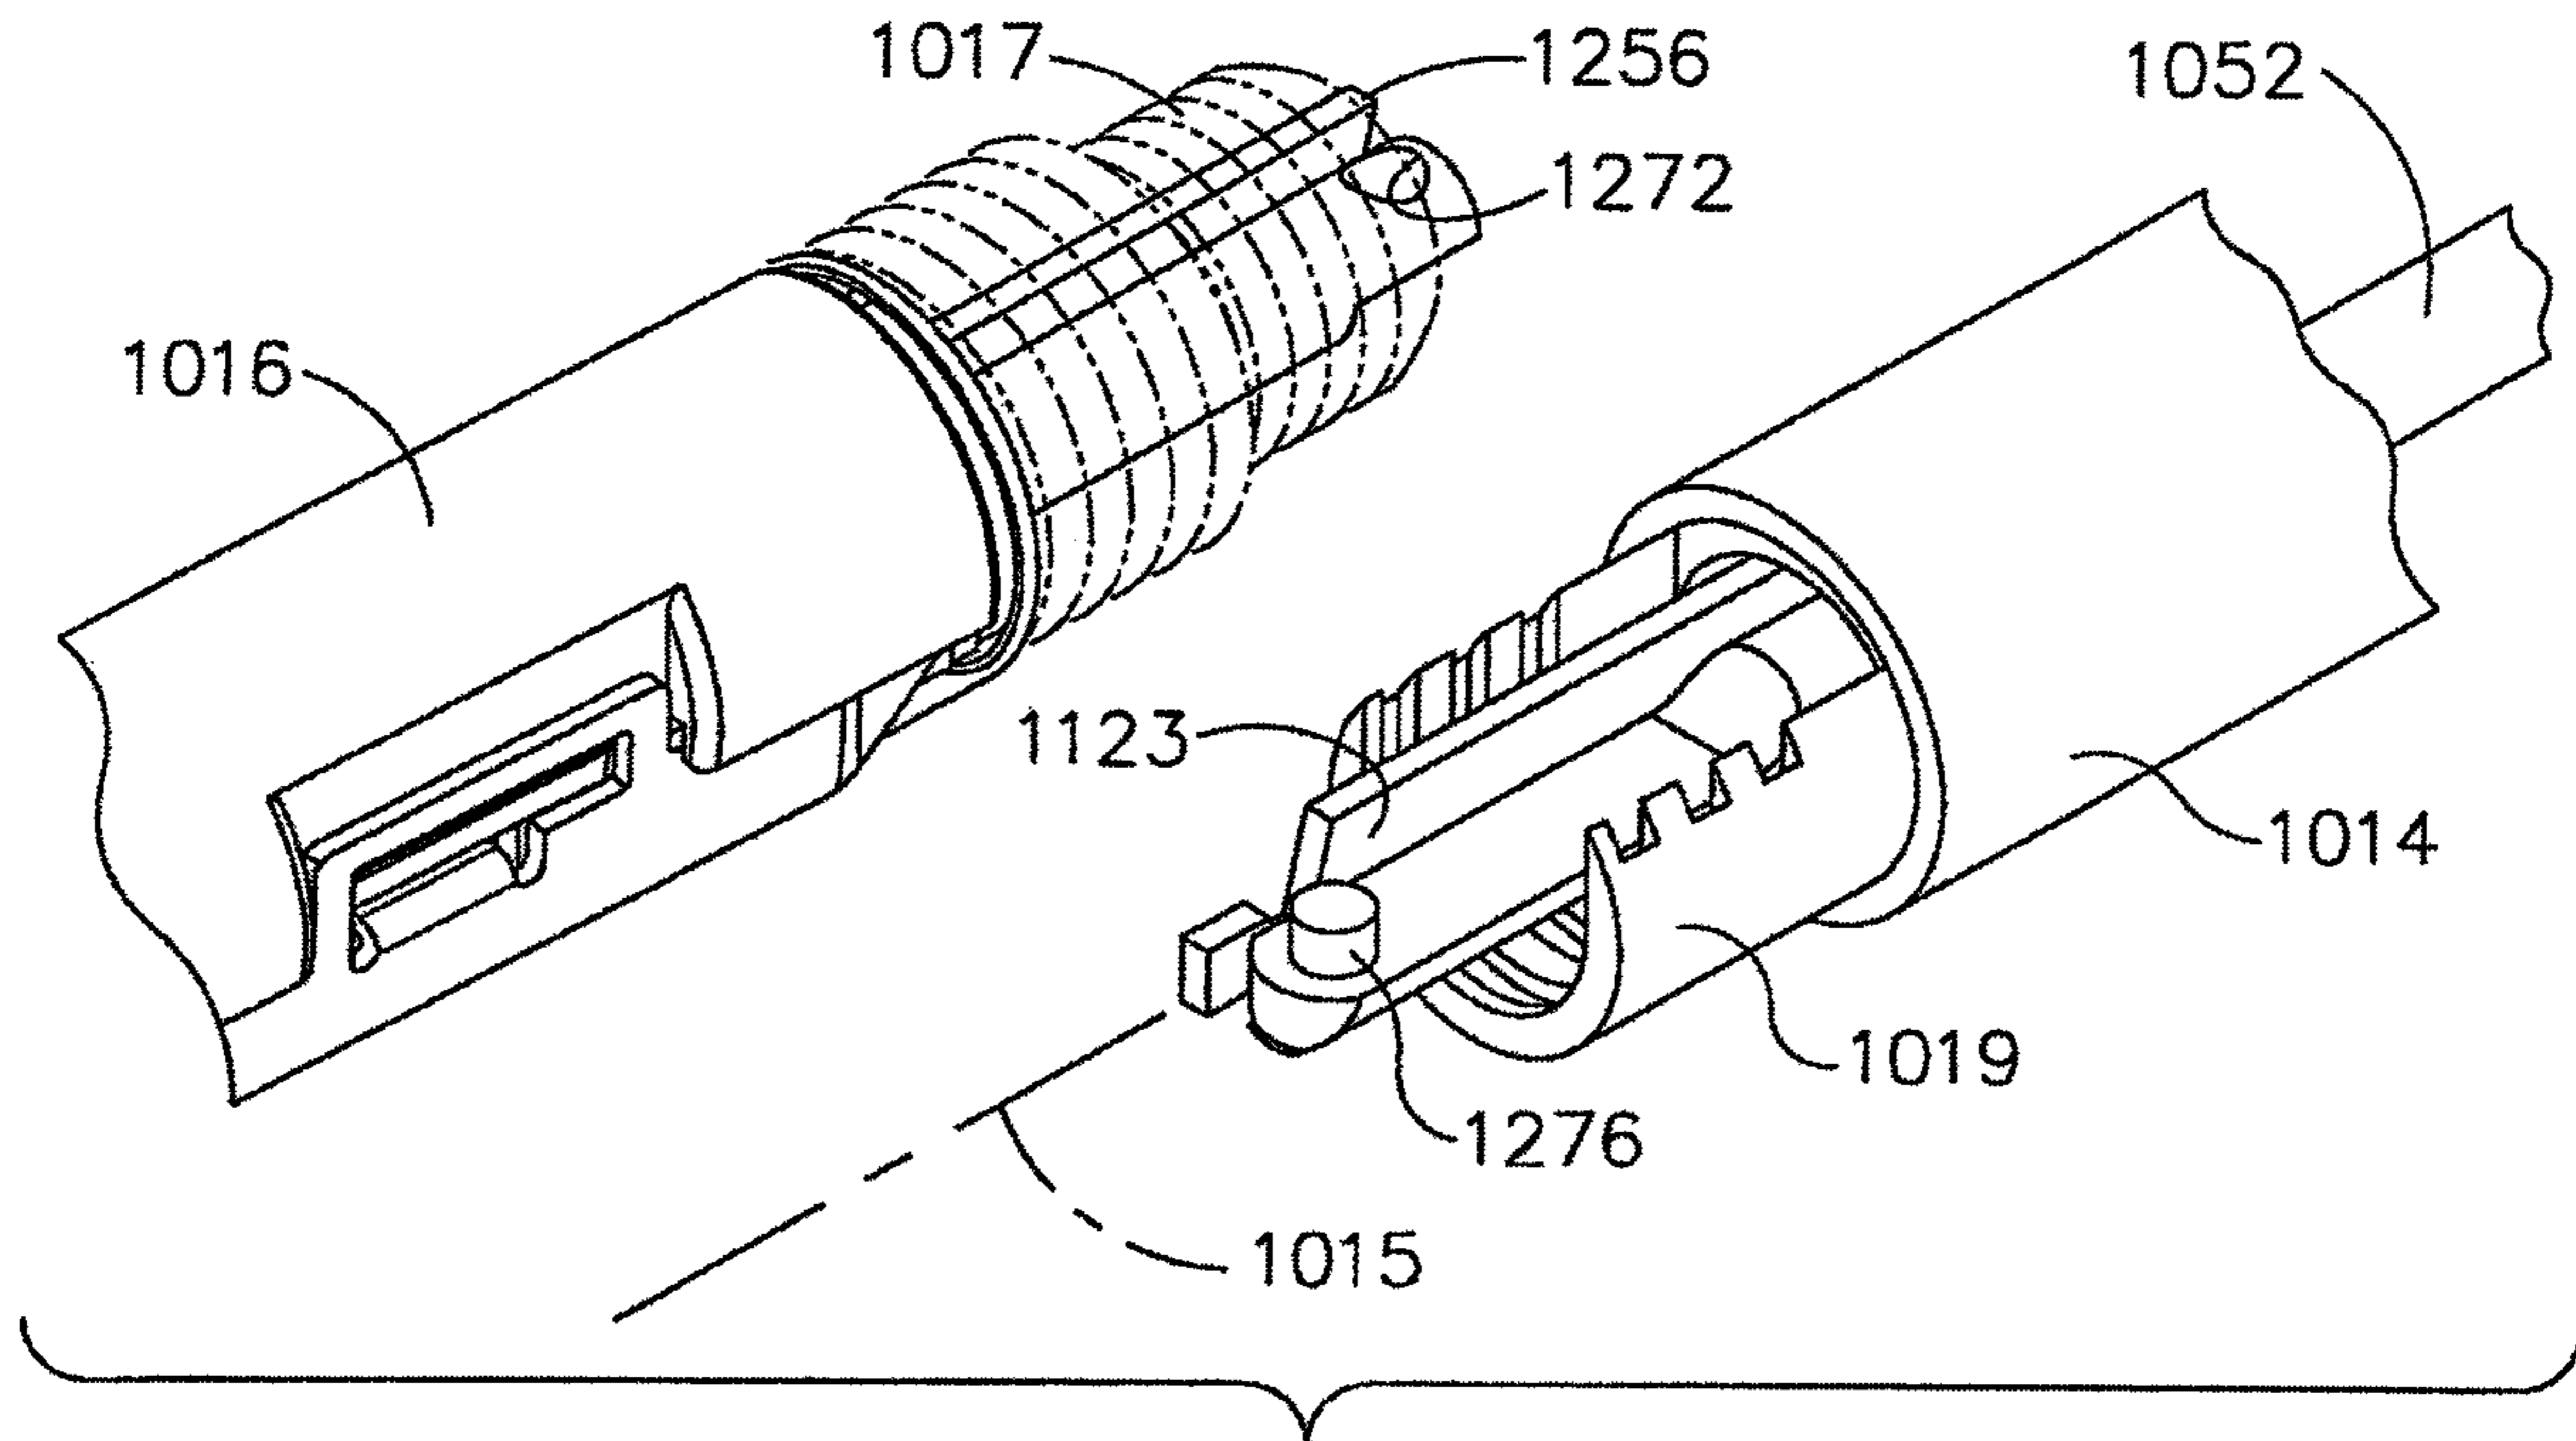


FIG. 66

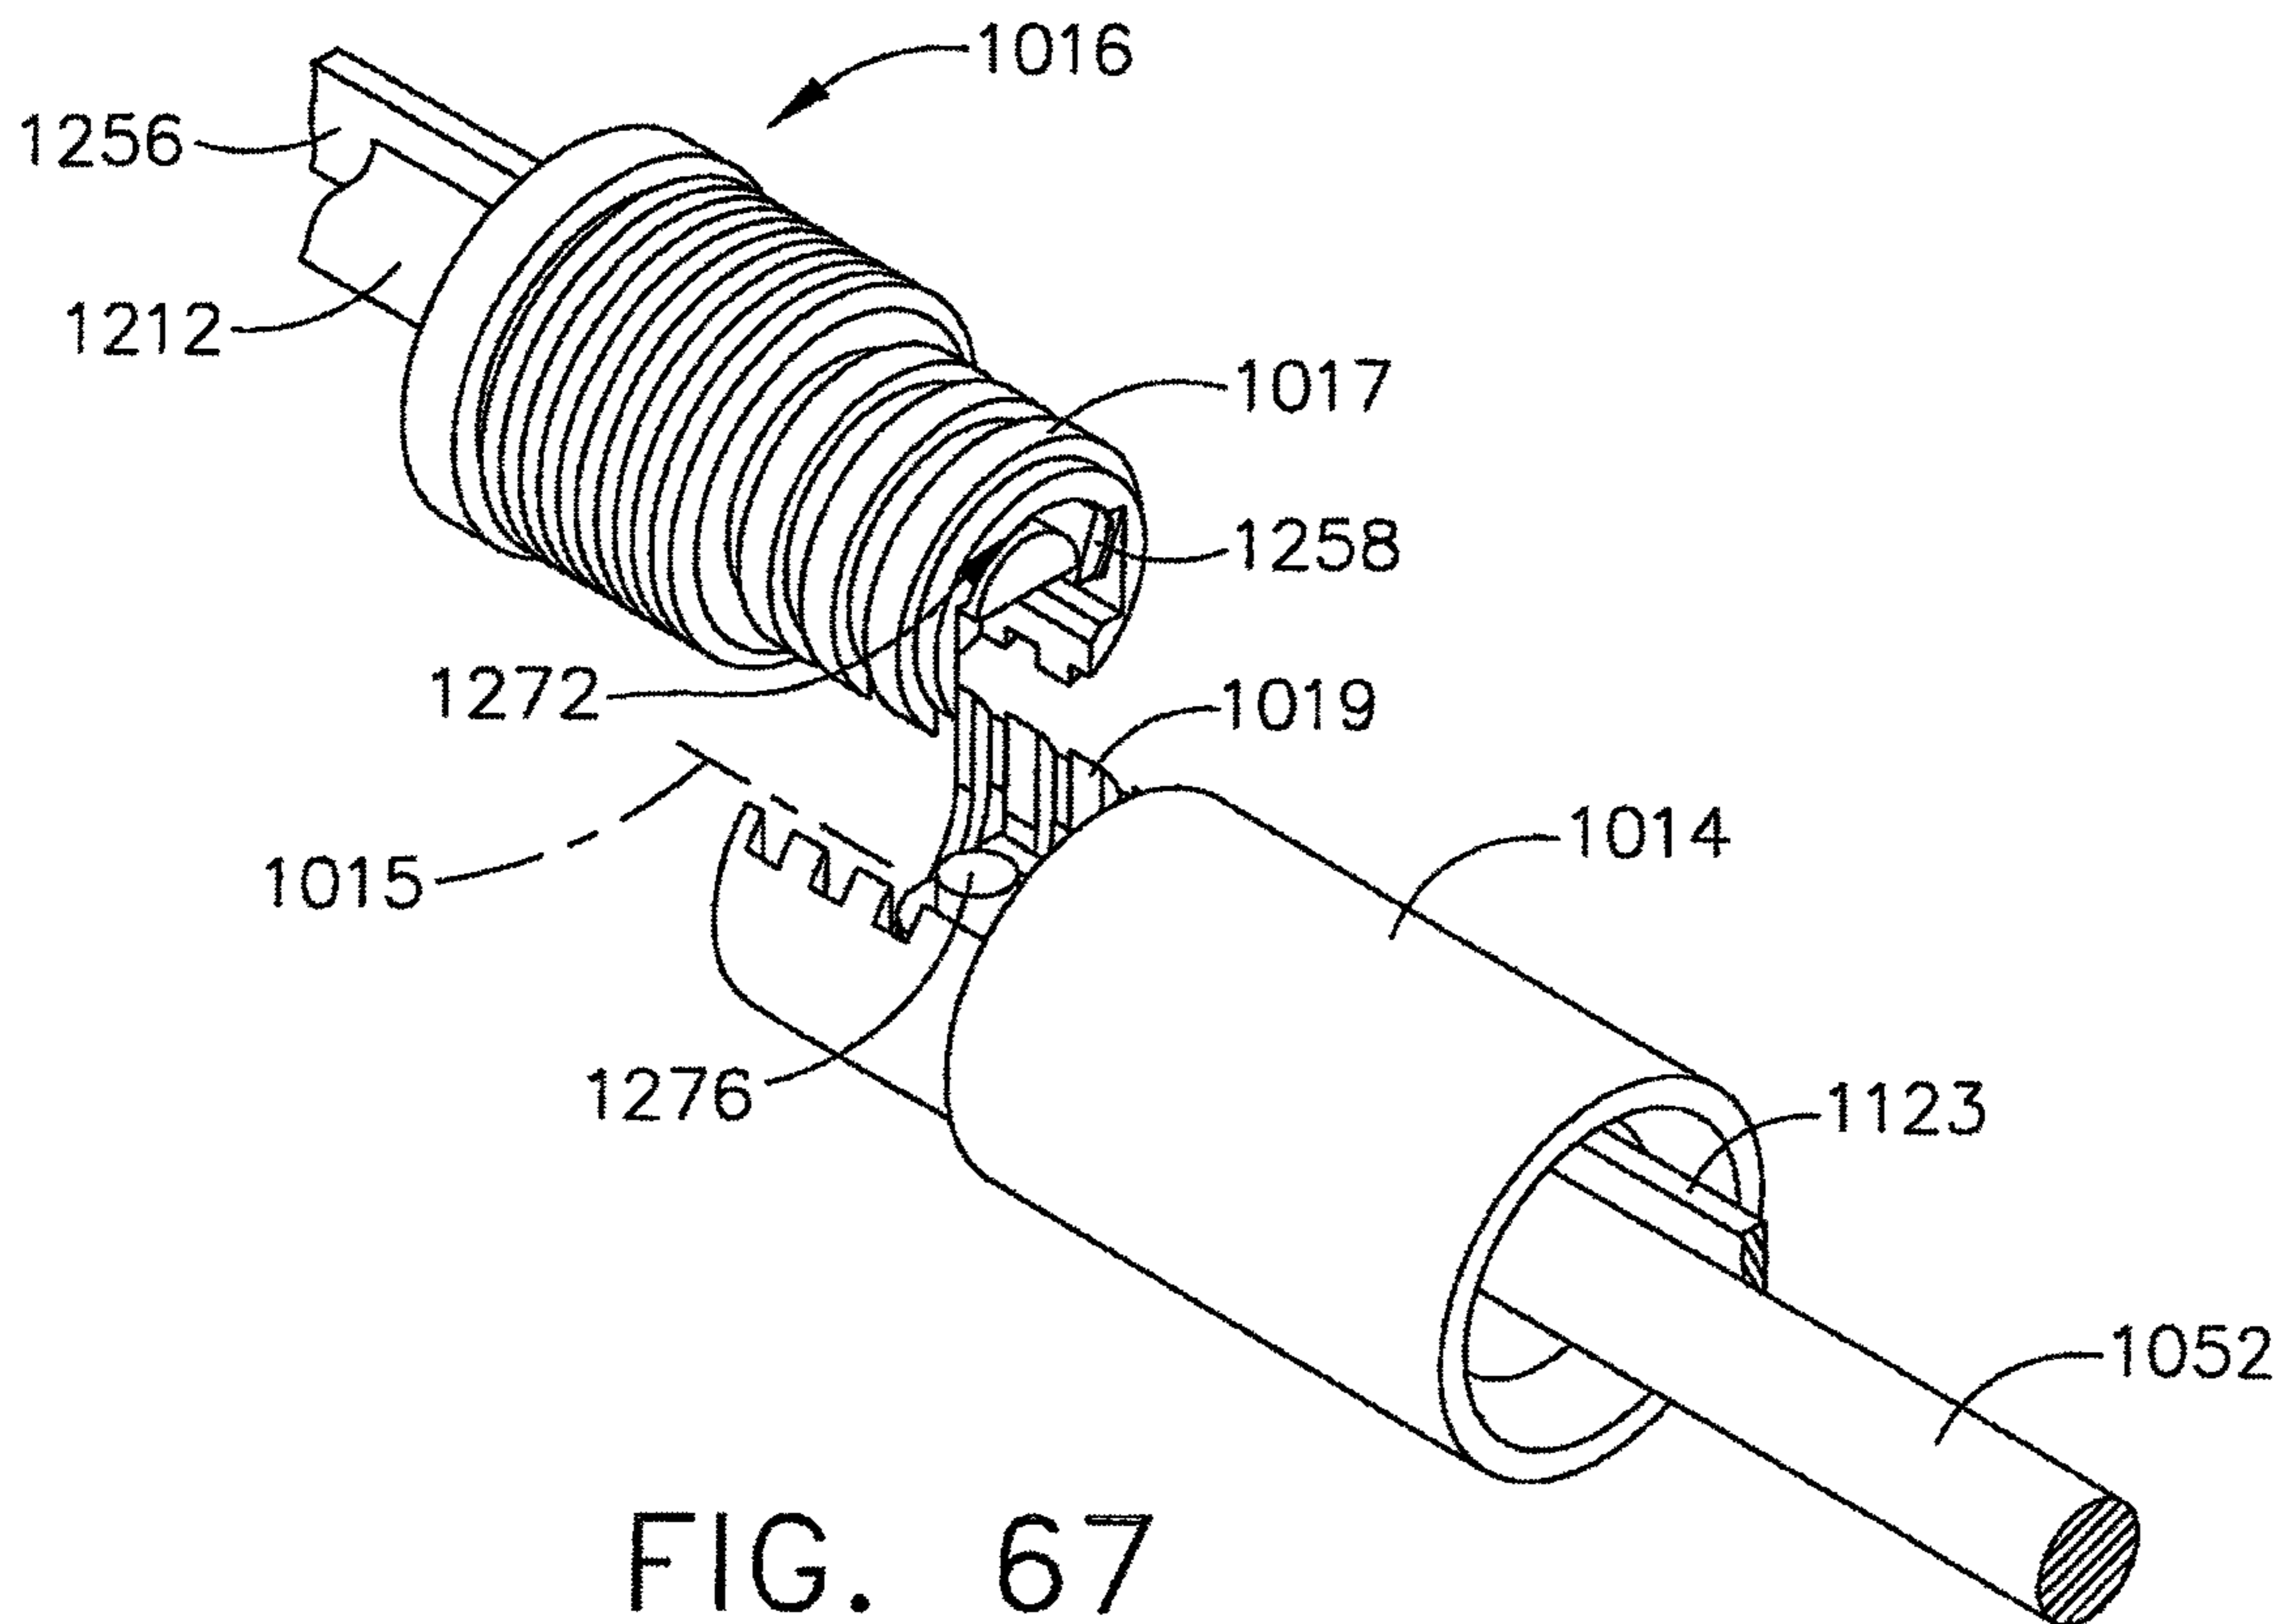


FIG. 67

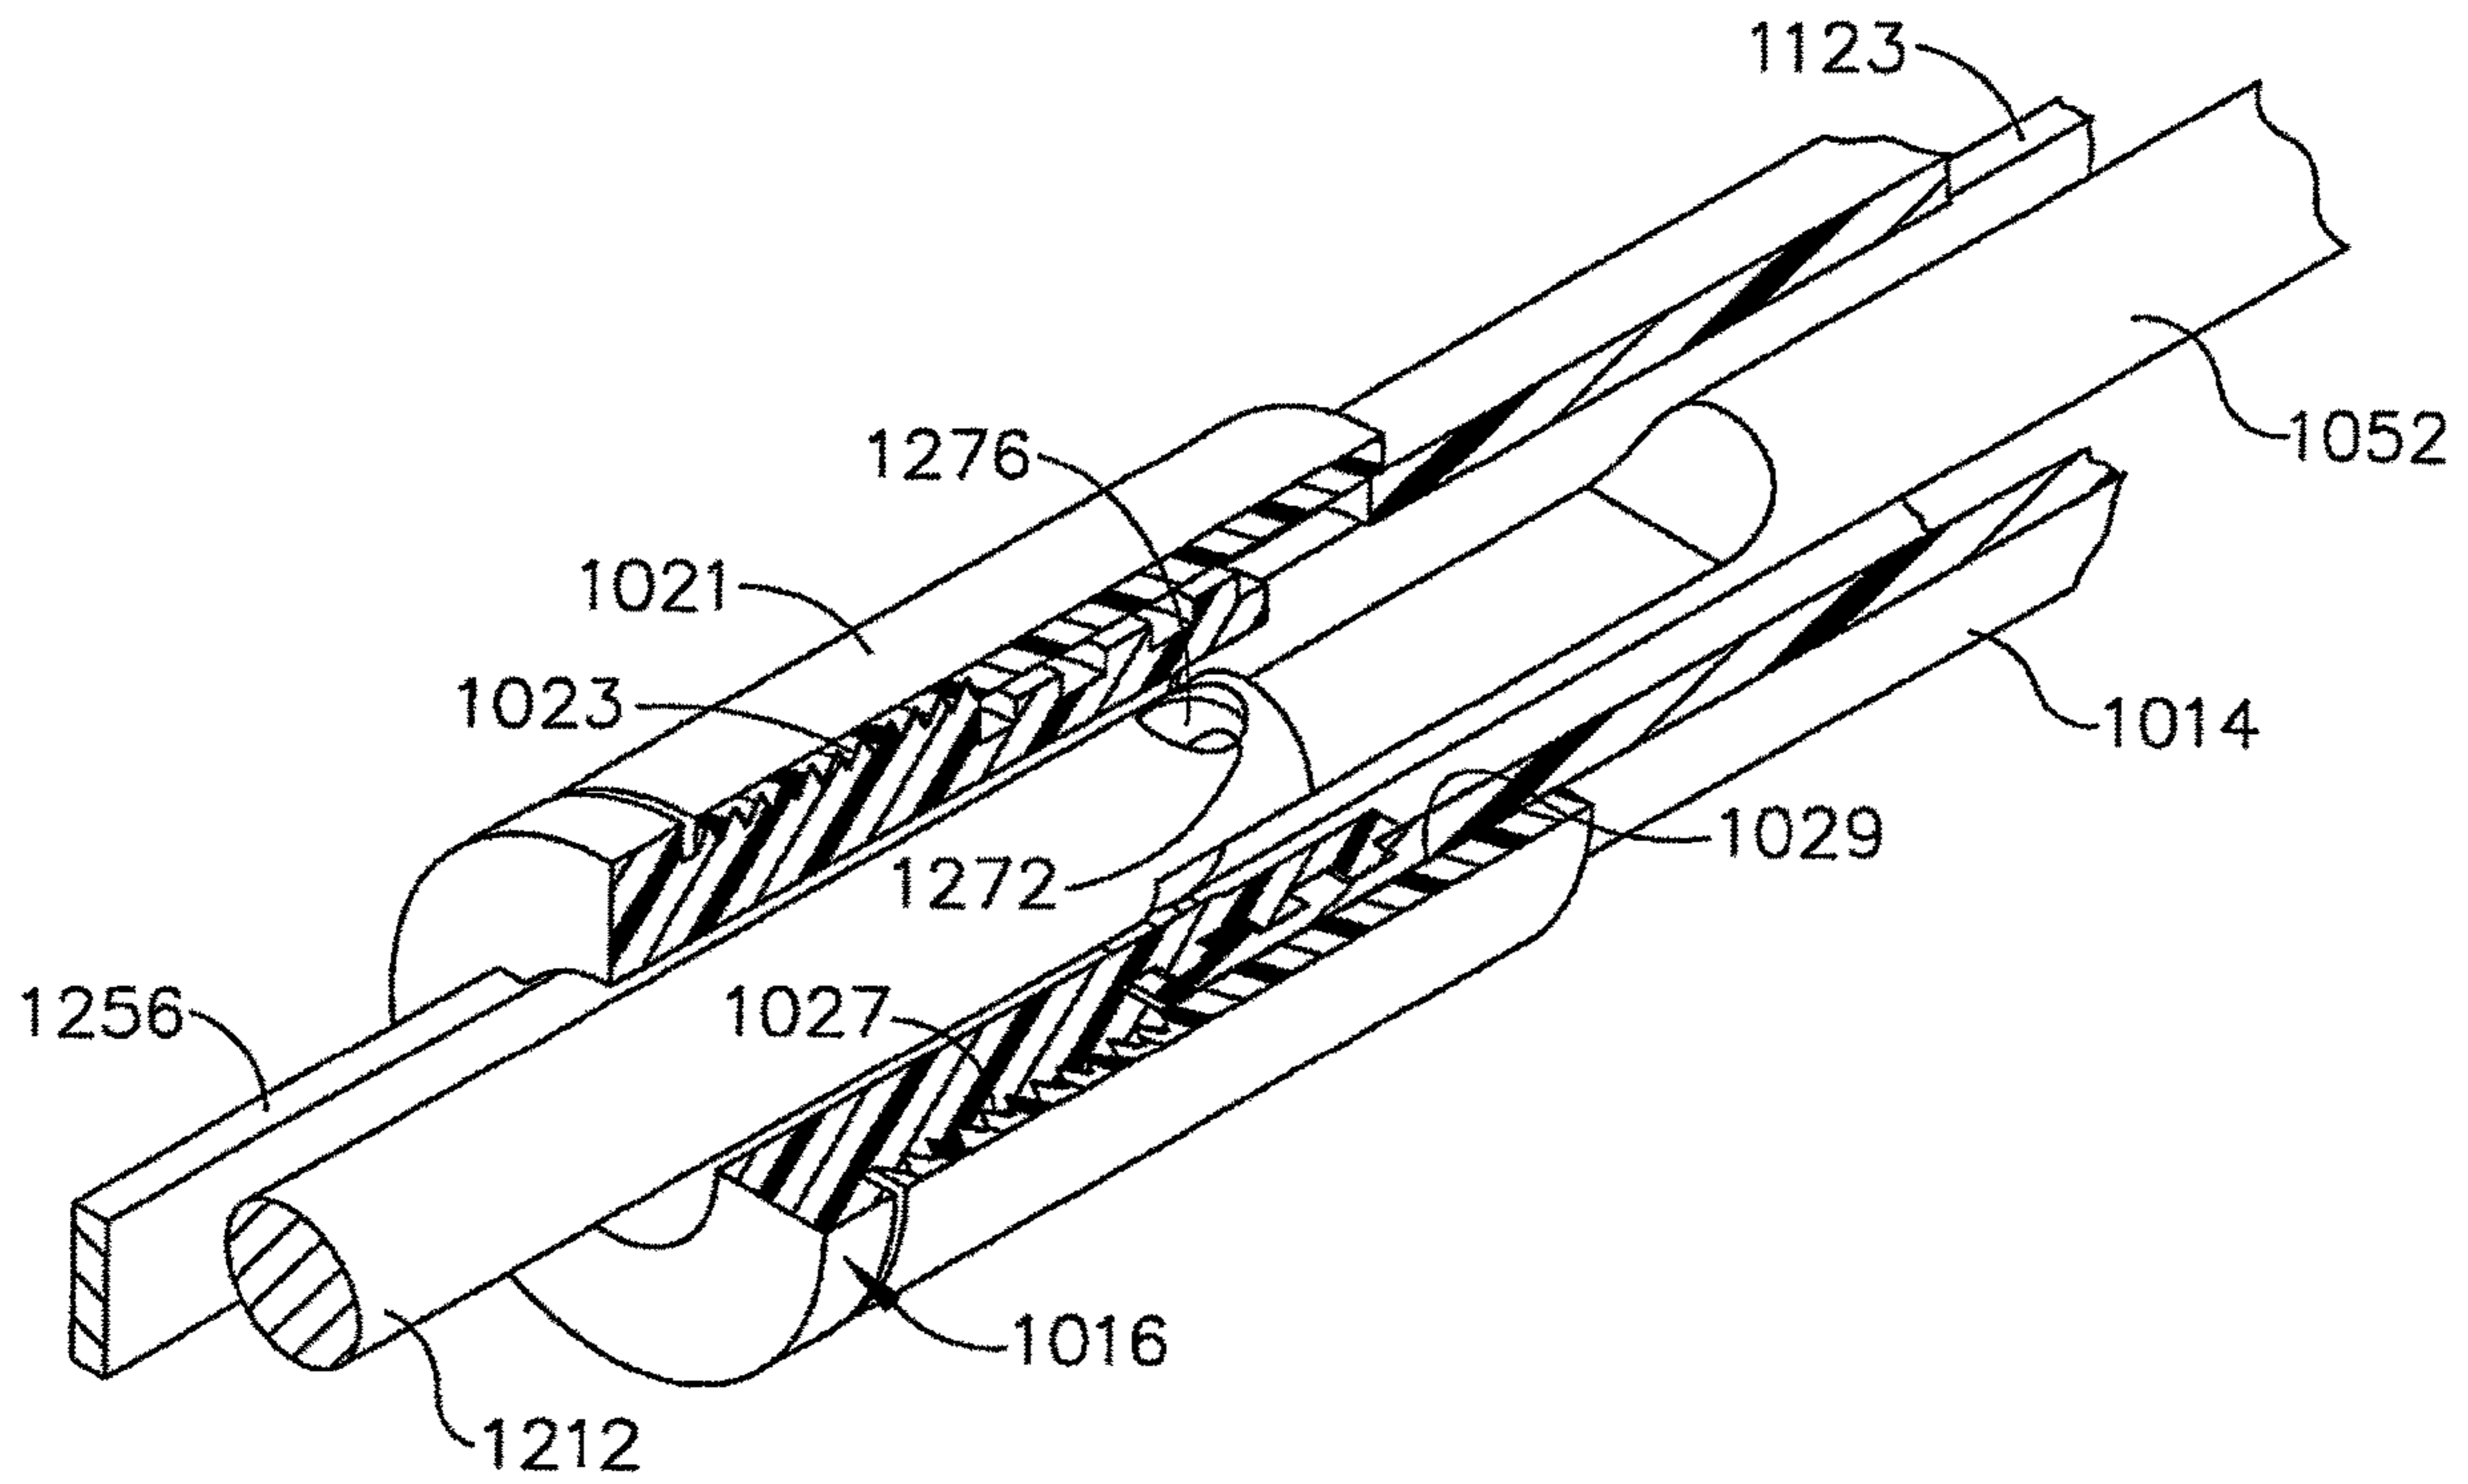


FIG. 68

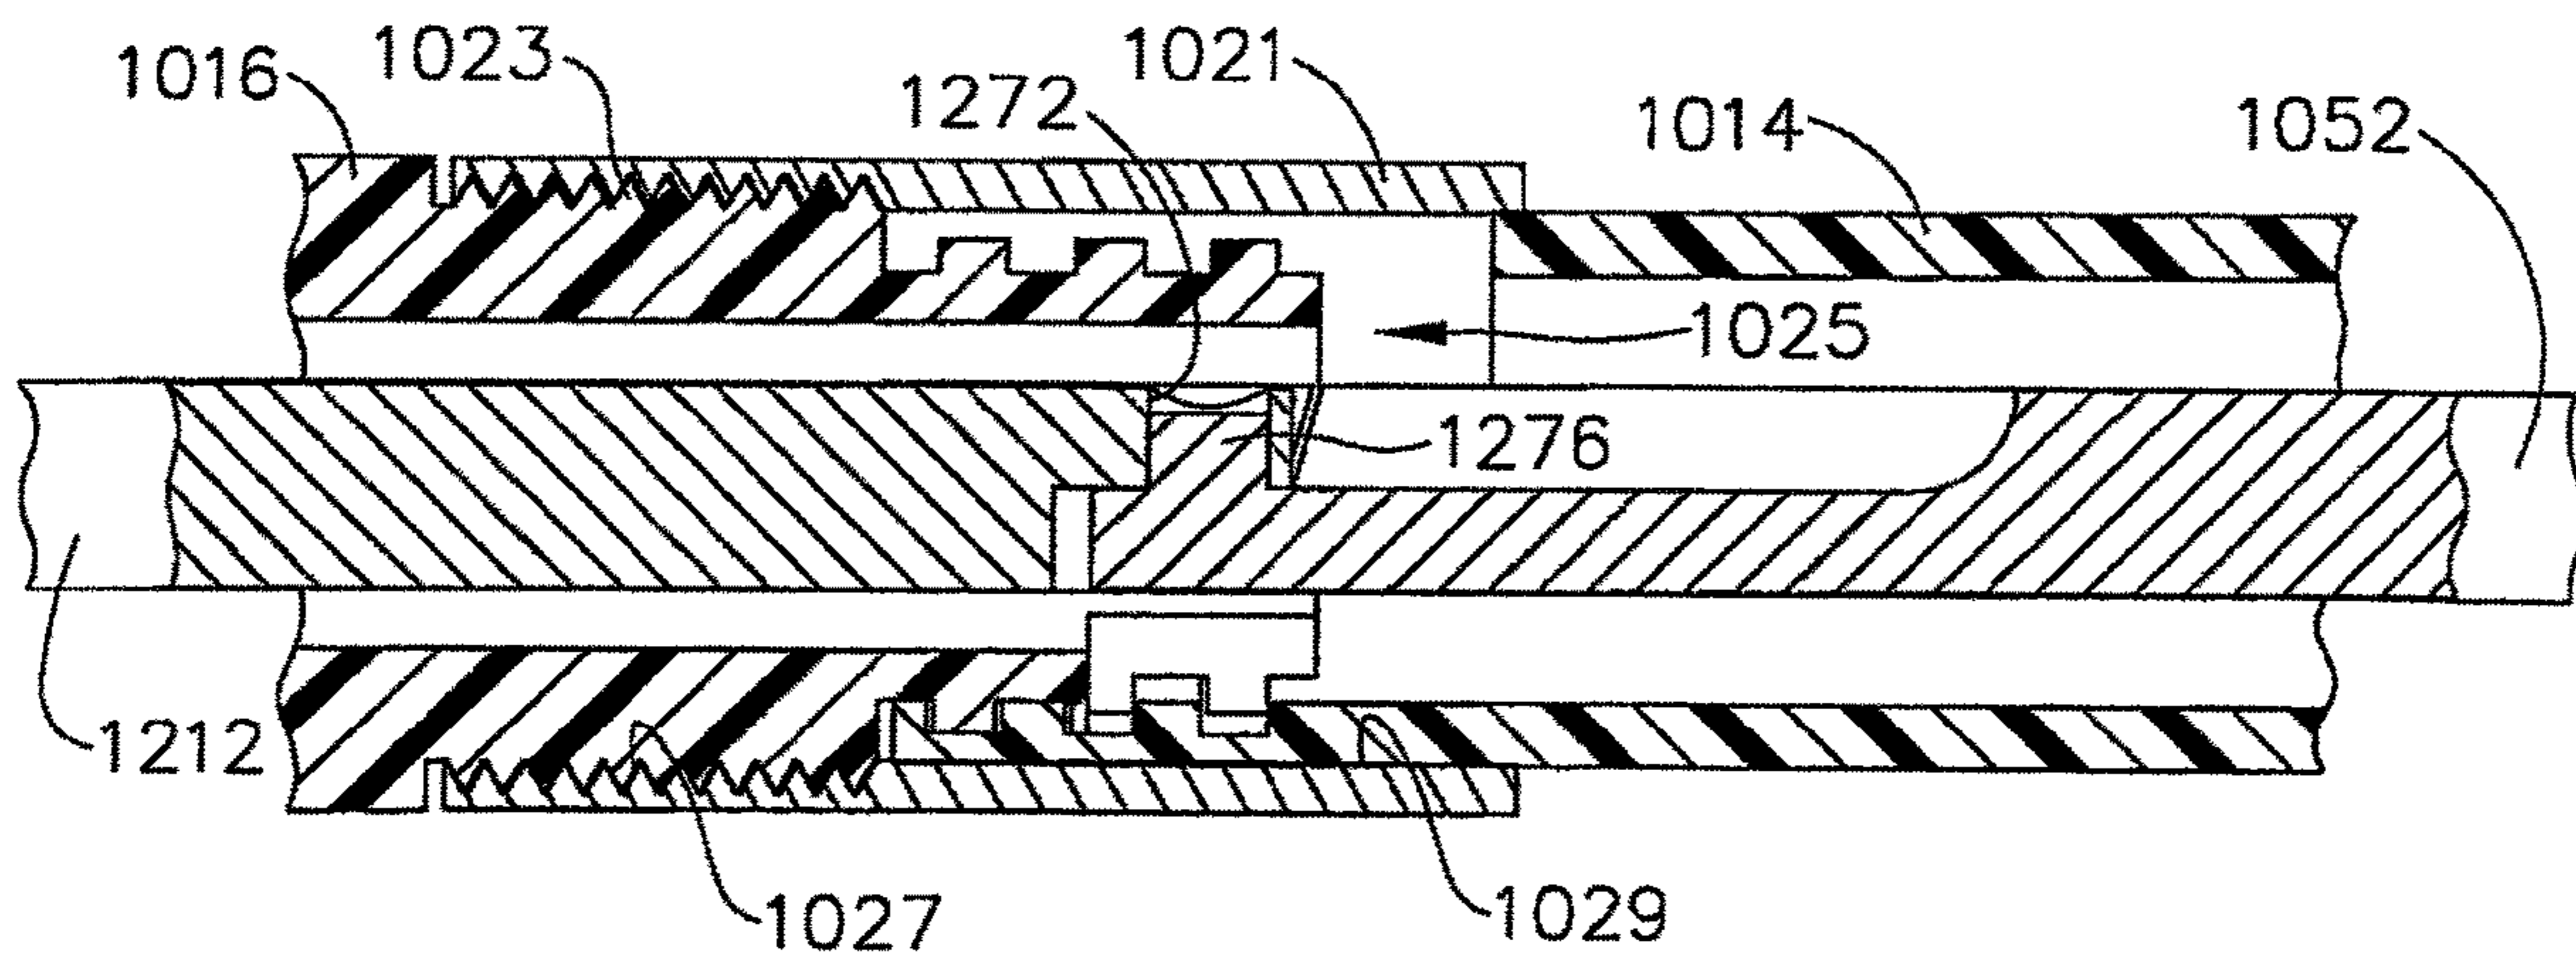


FIG. 69

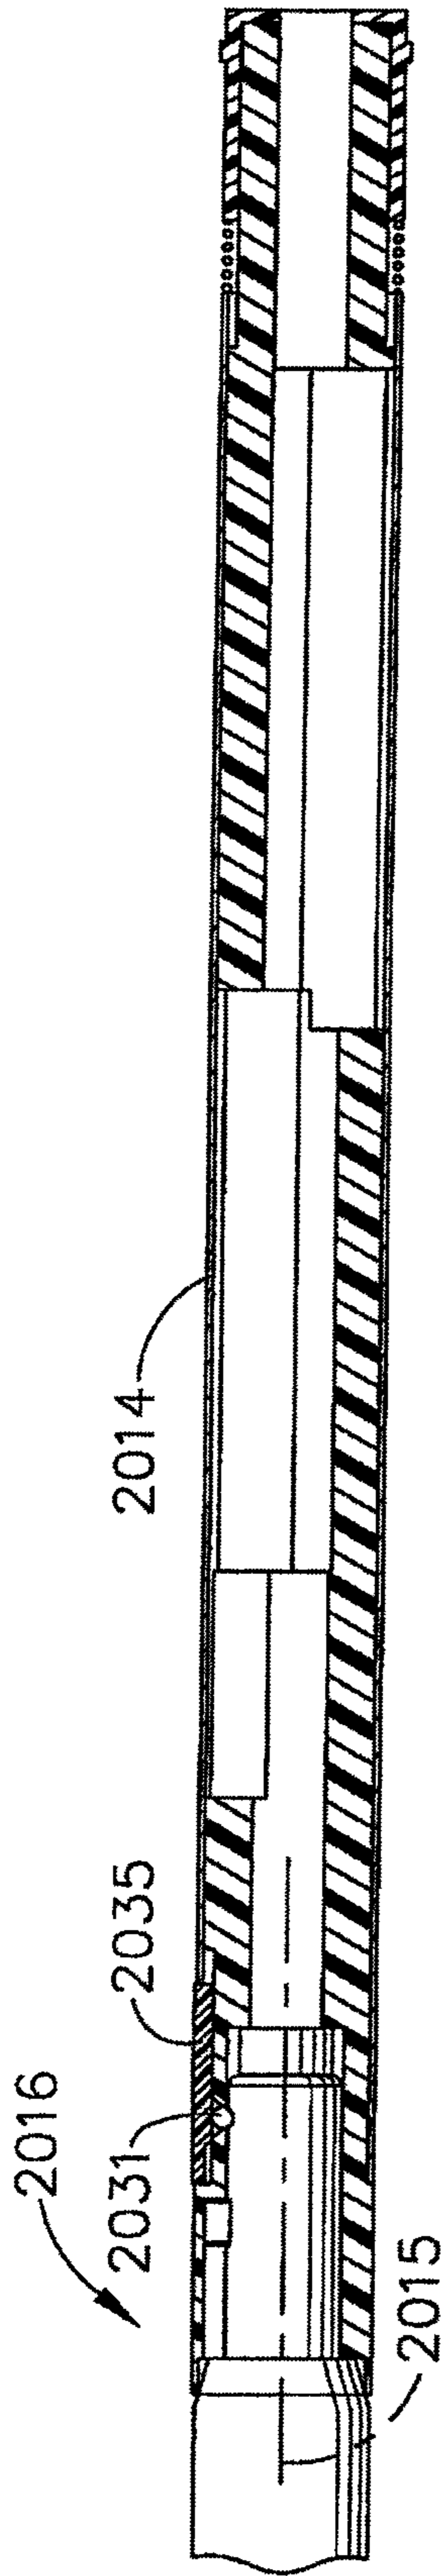


FIG. 70

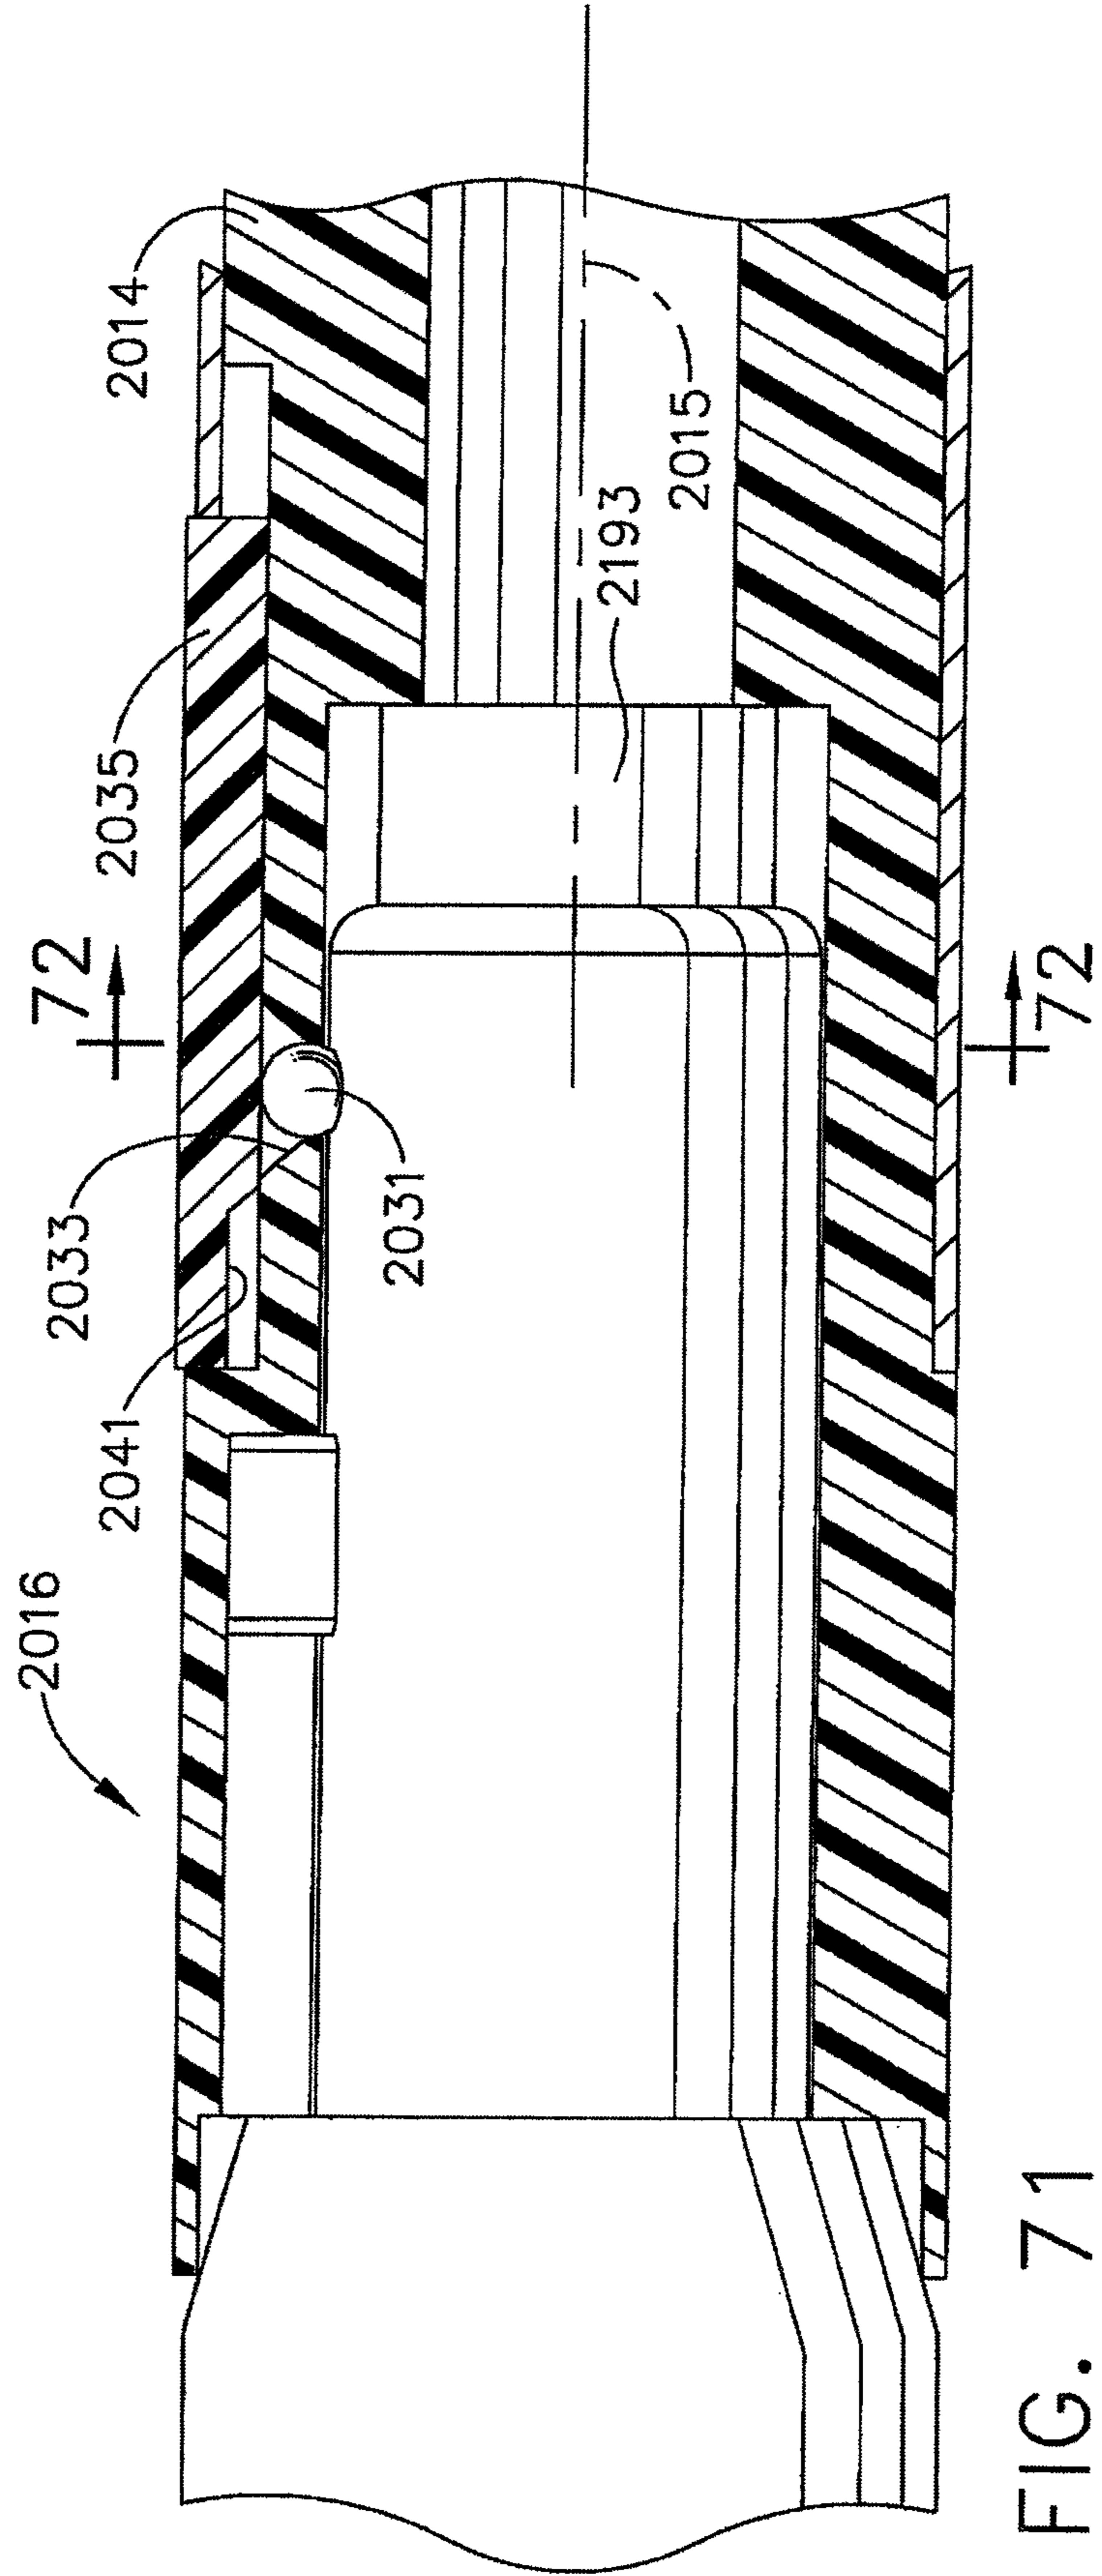


FIG. 71

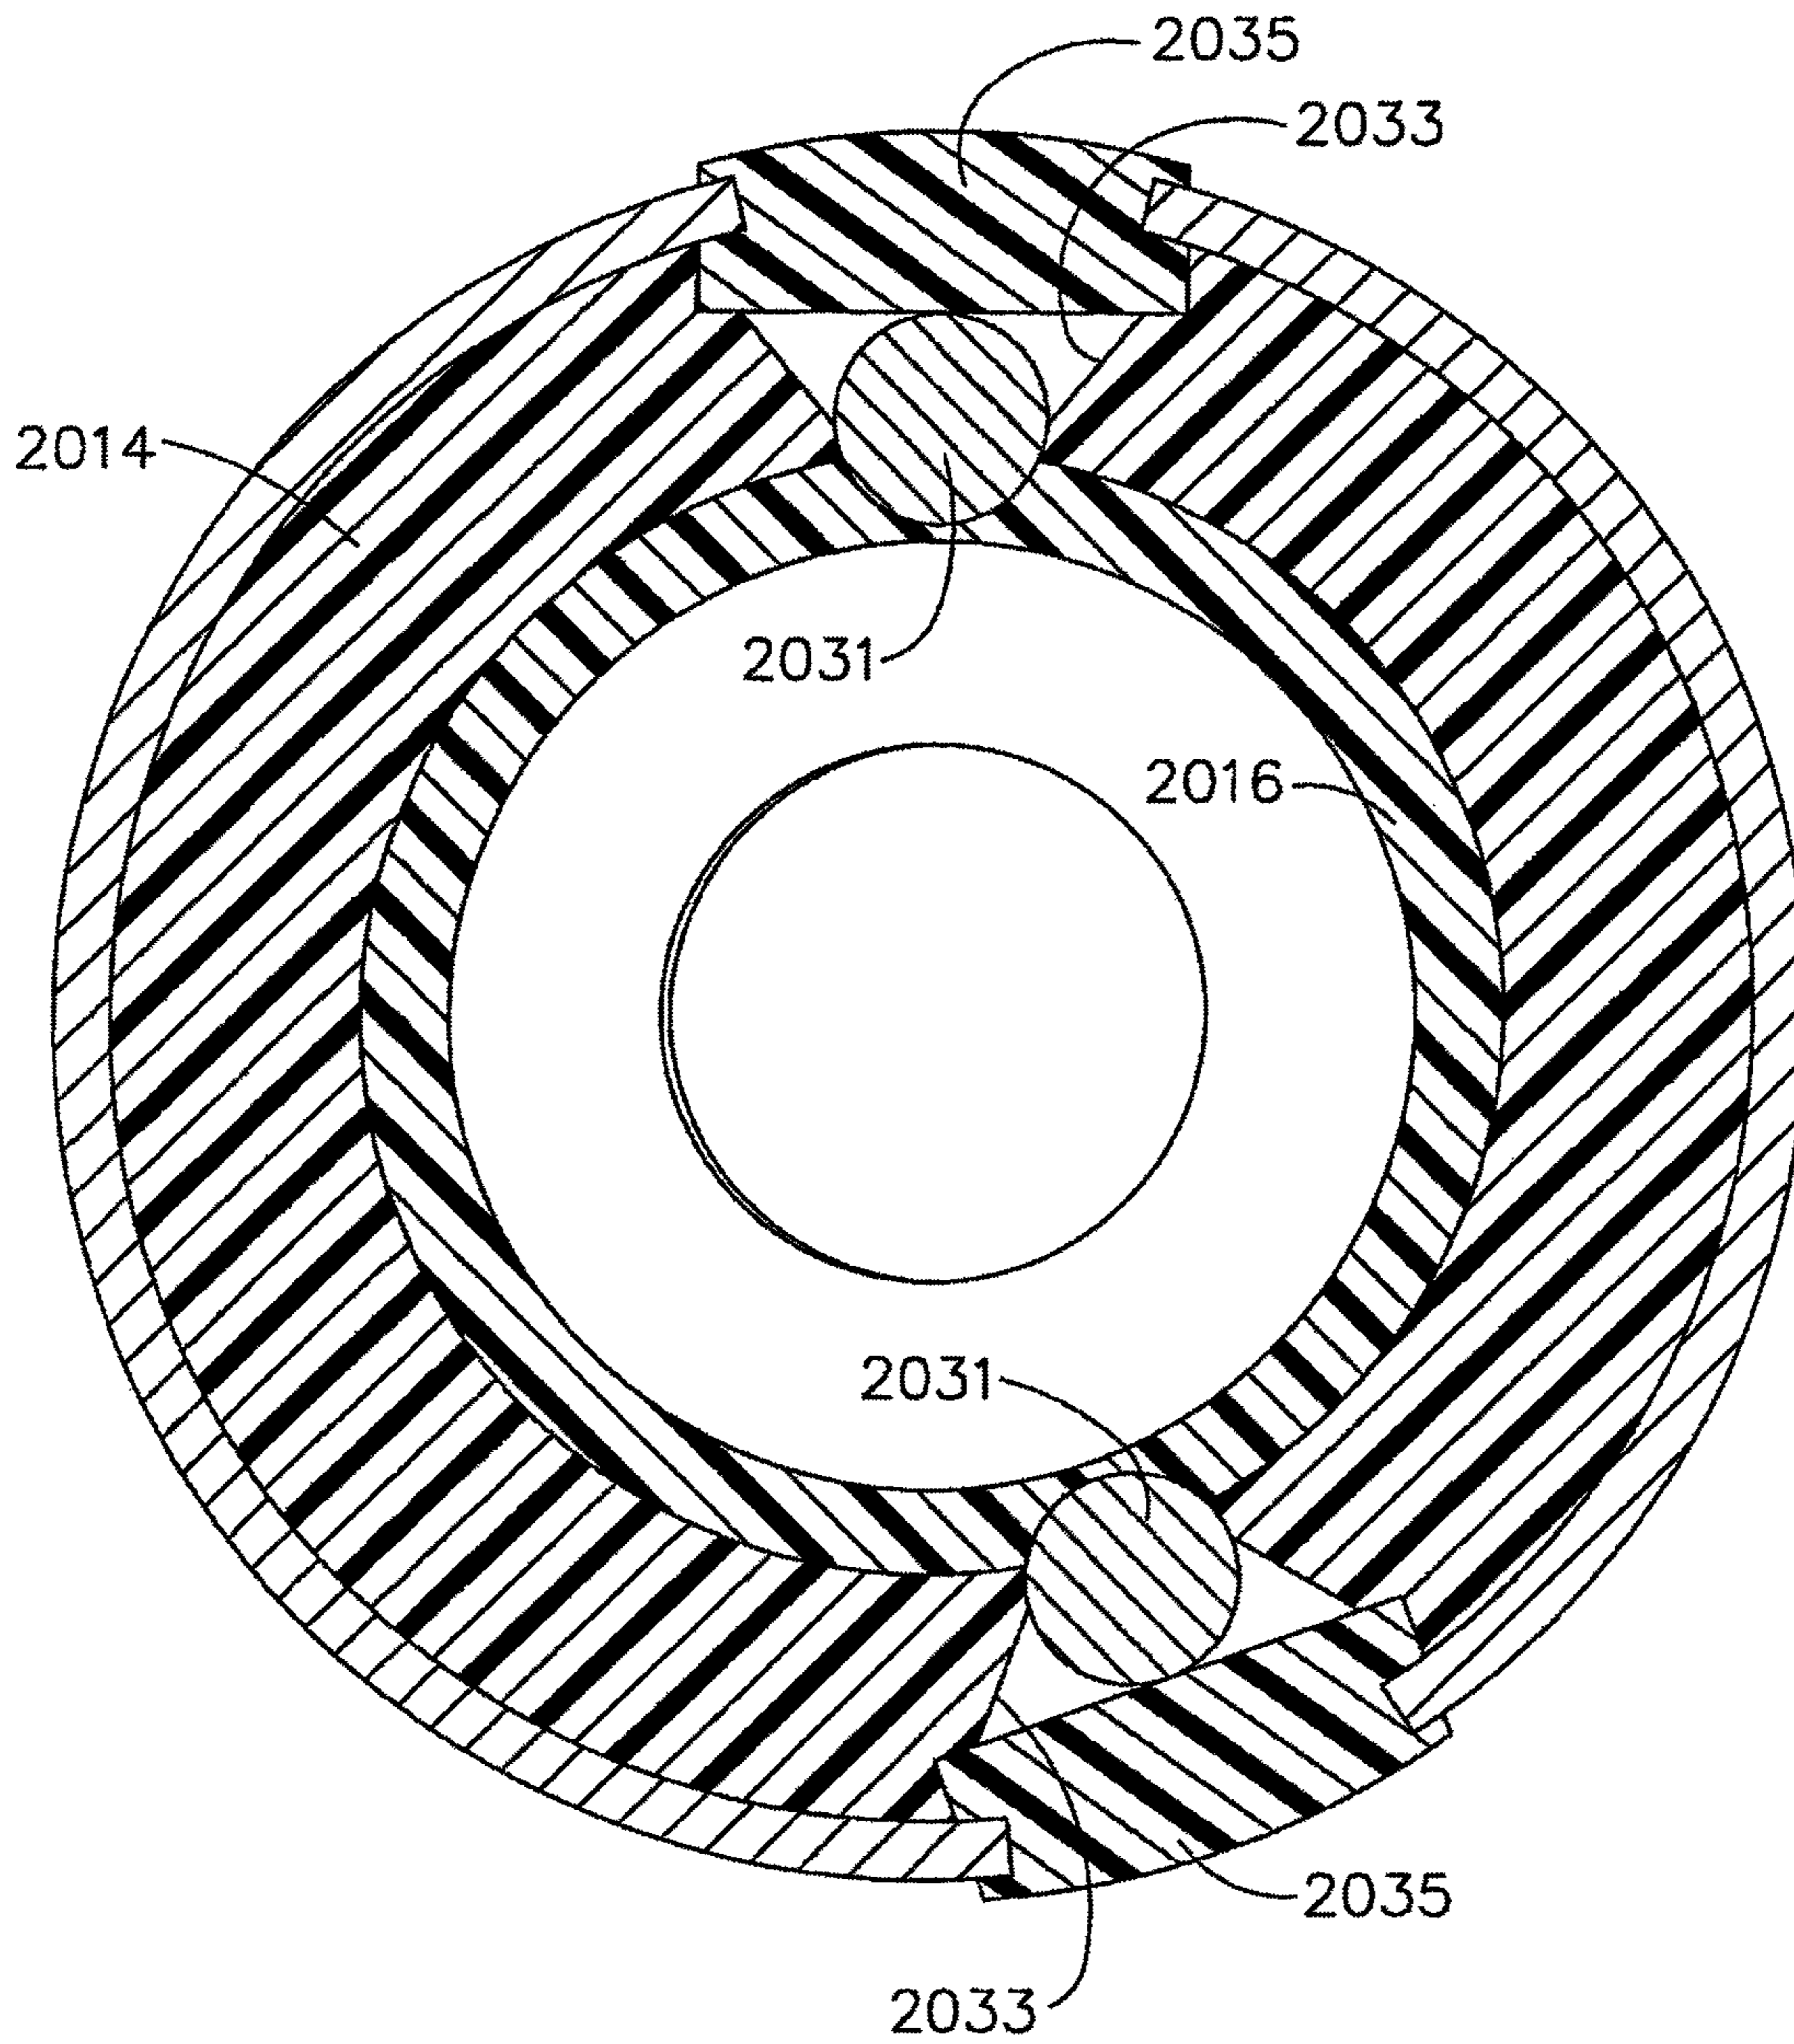


FIG. 72

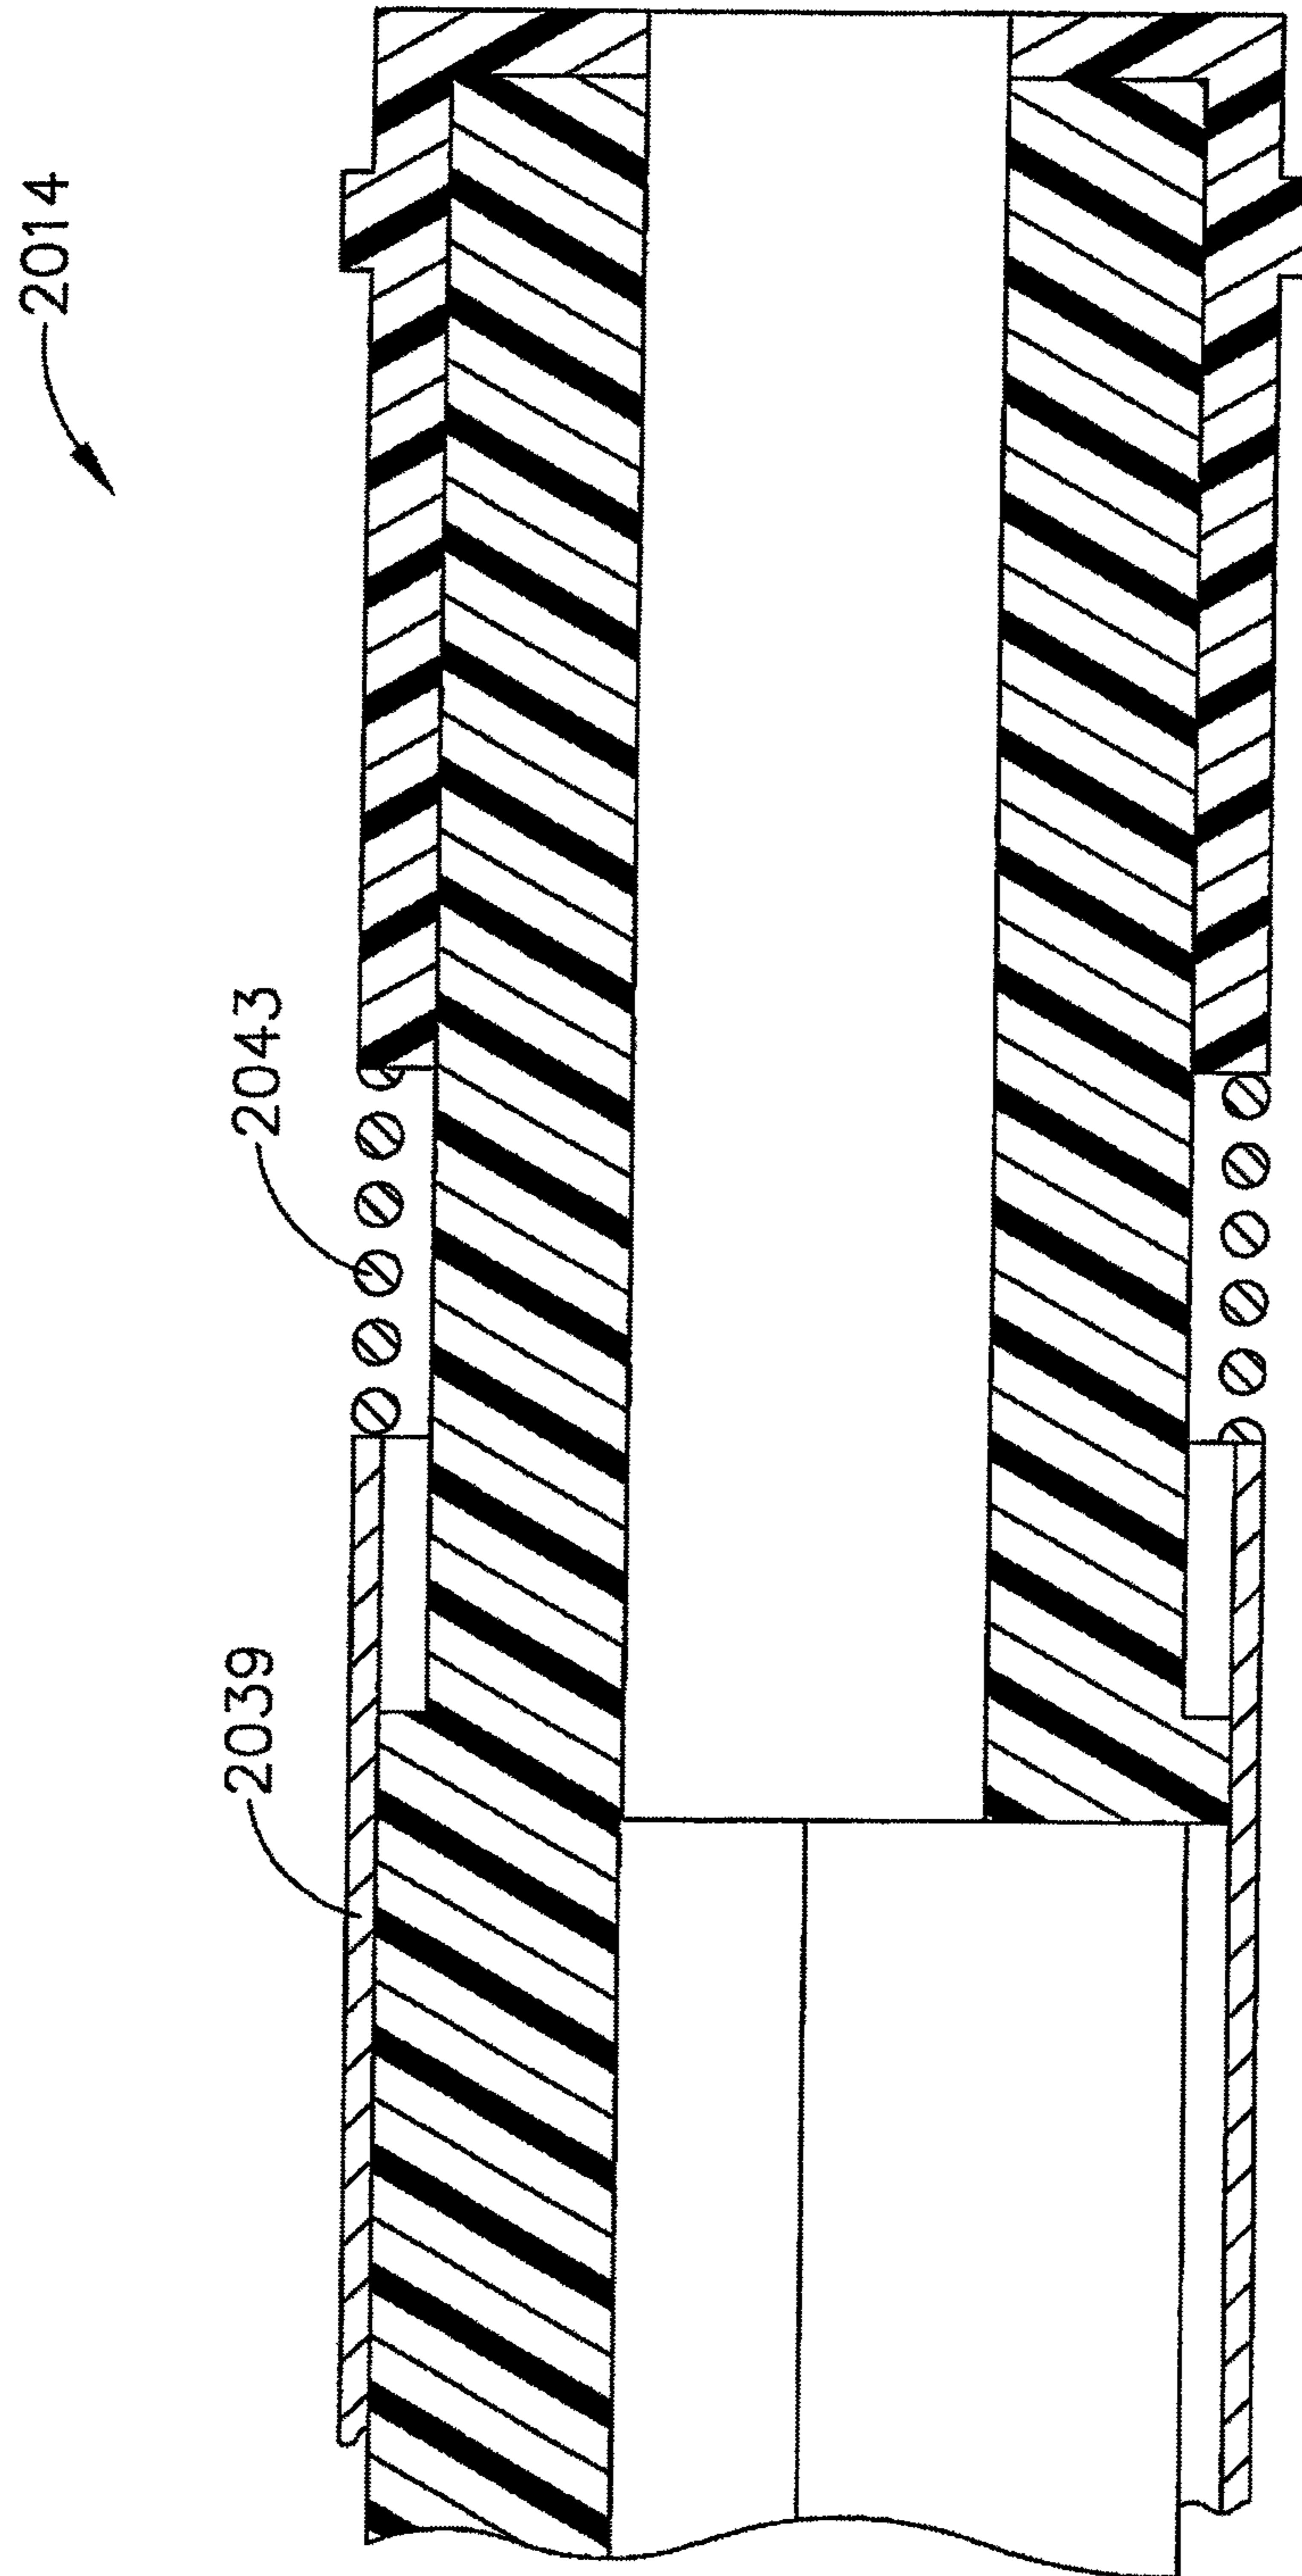


FIG. 73

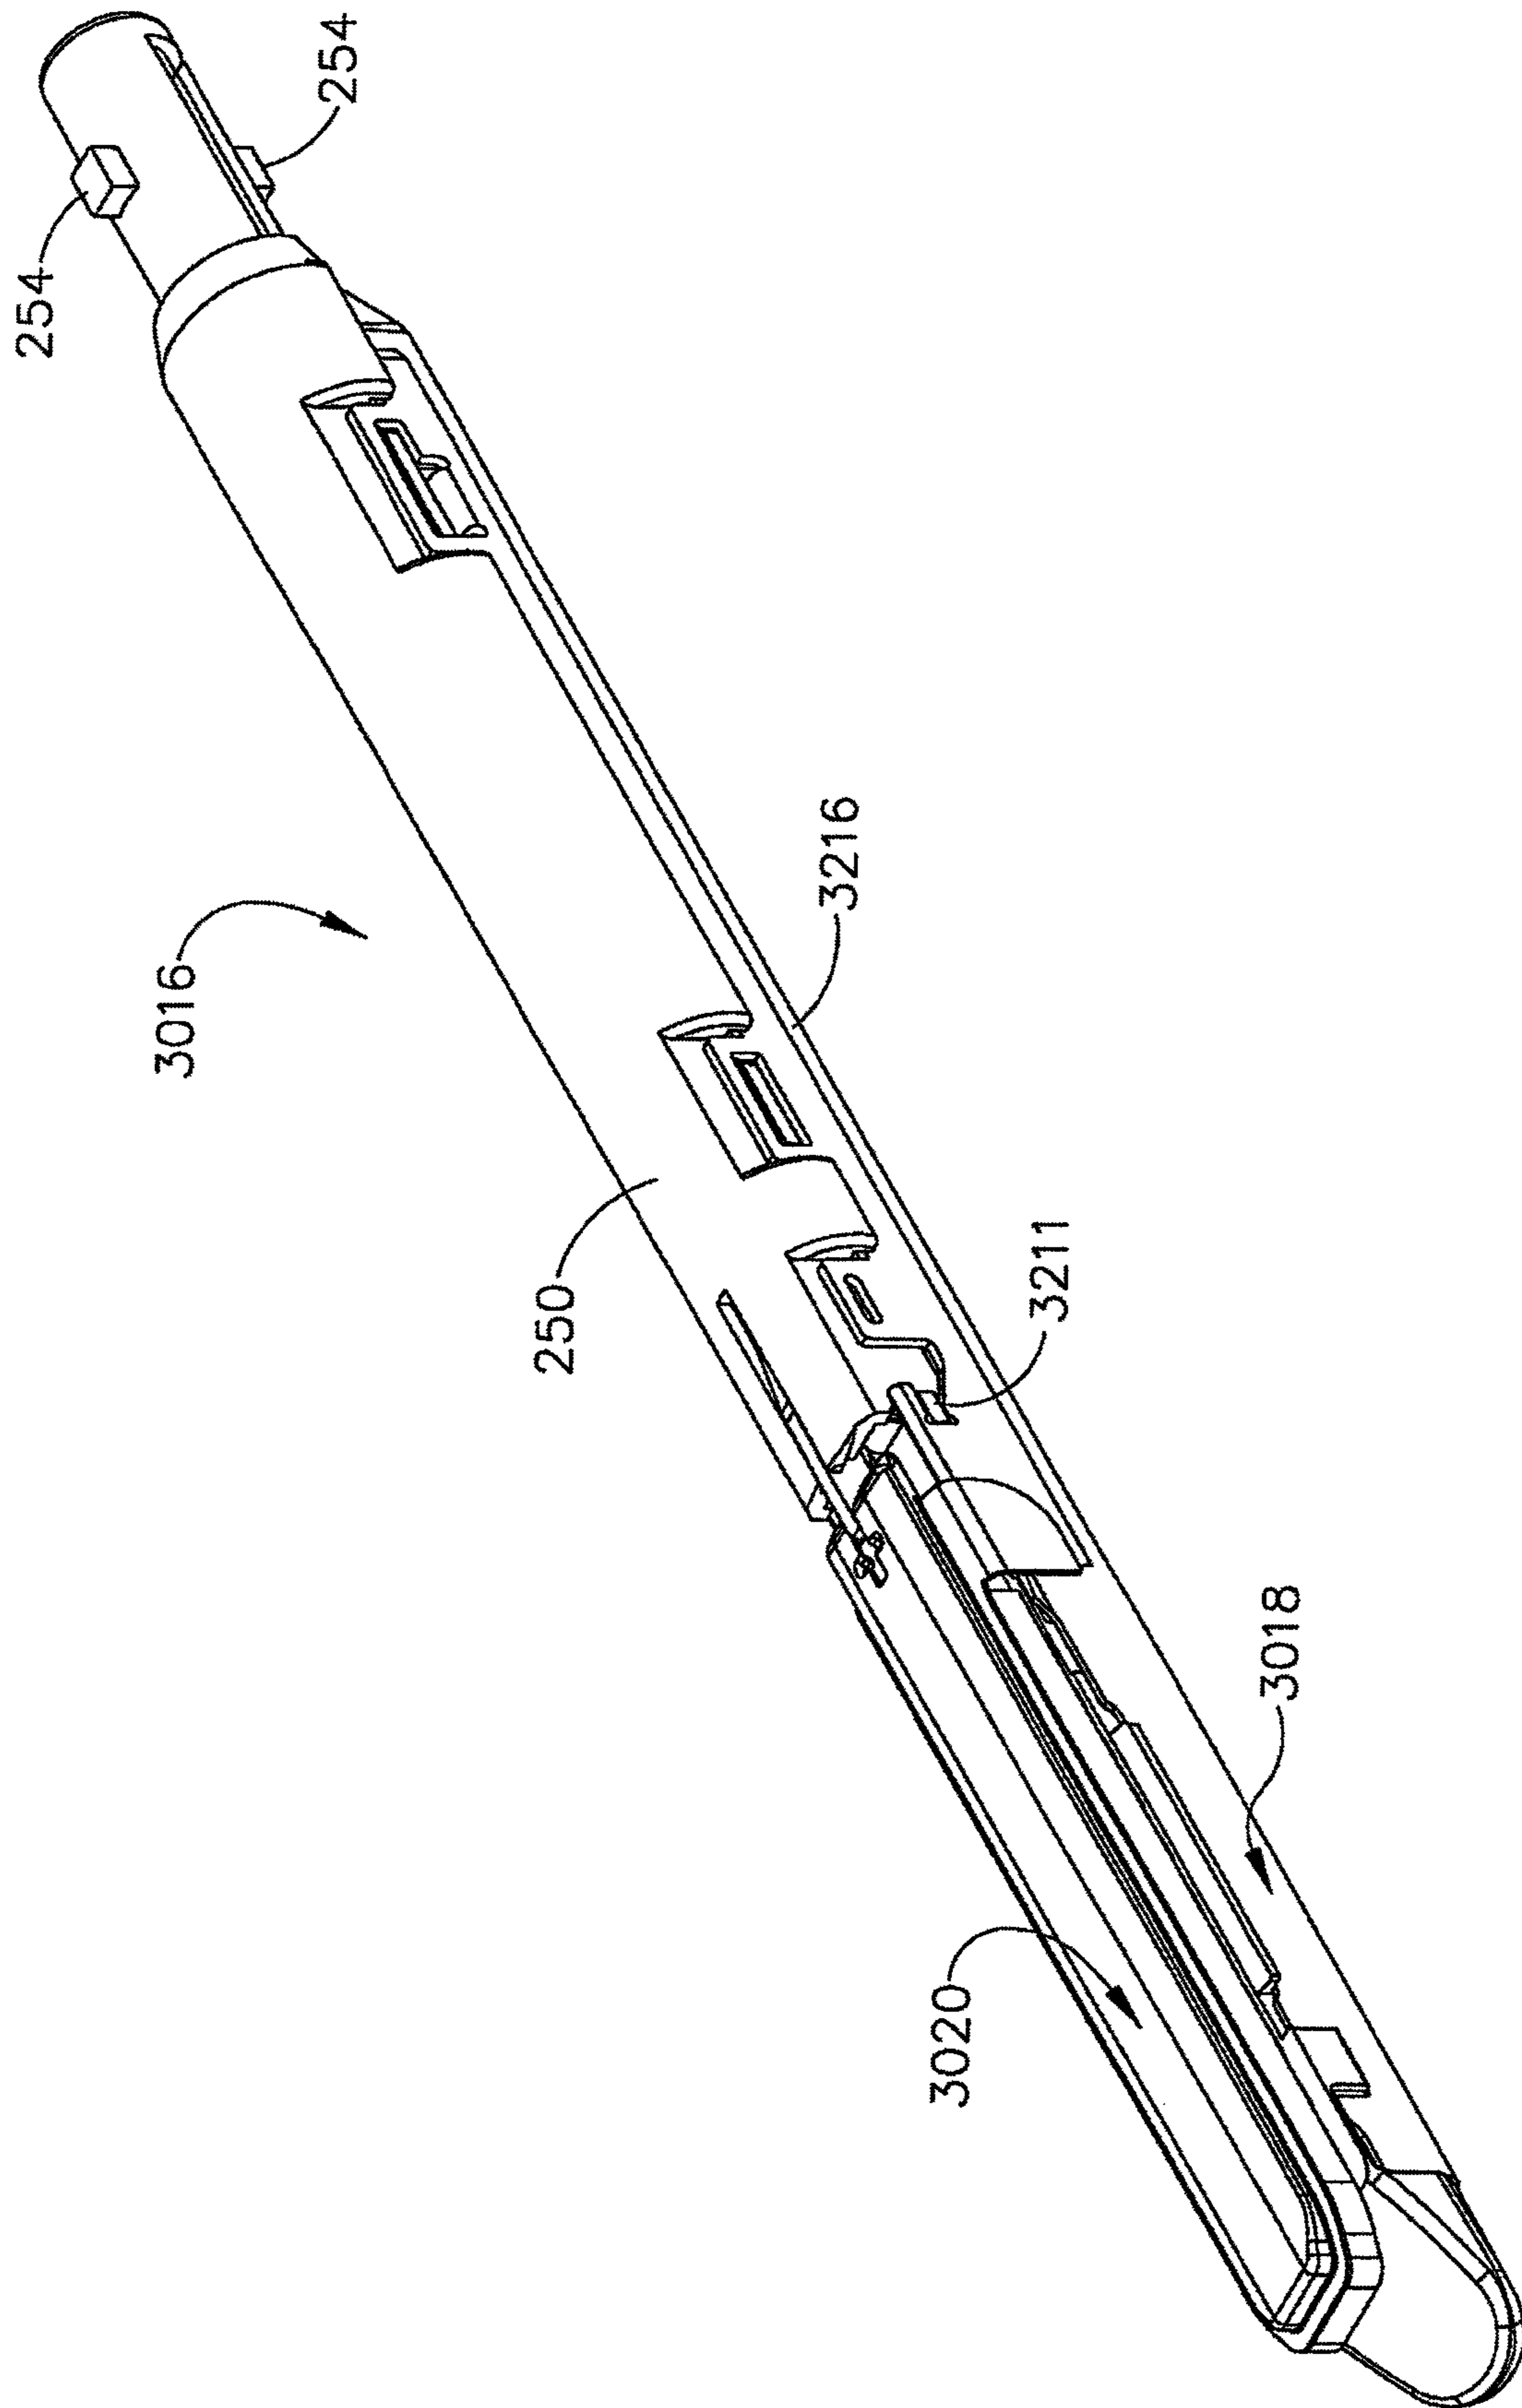


FIG. 74

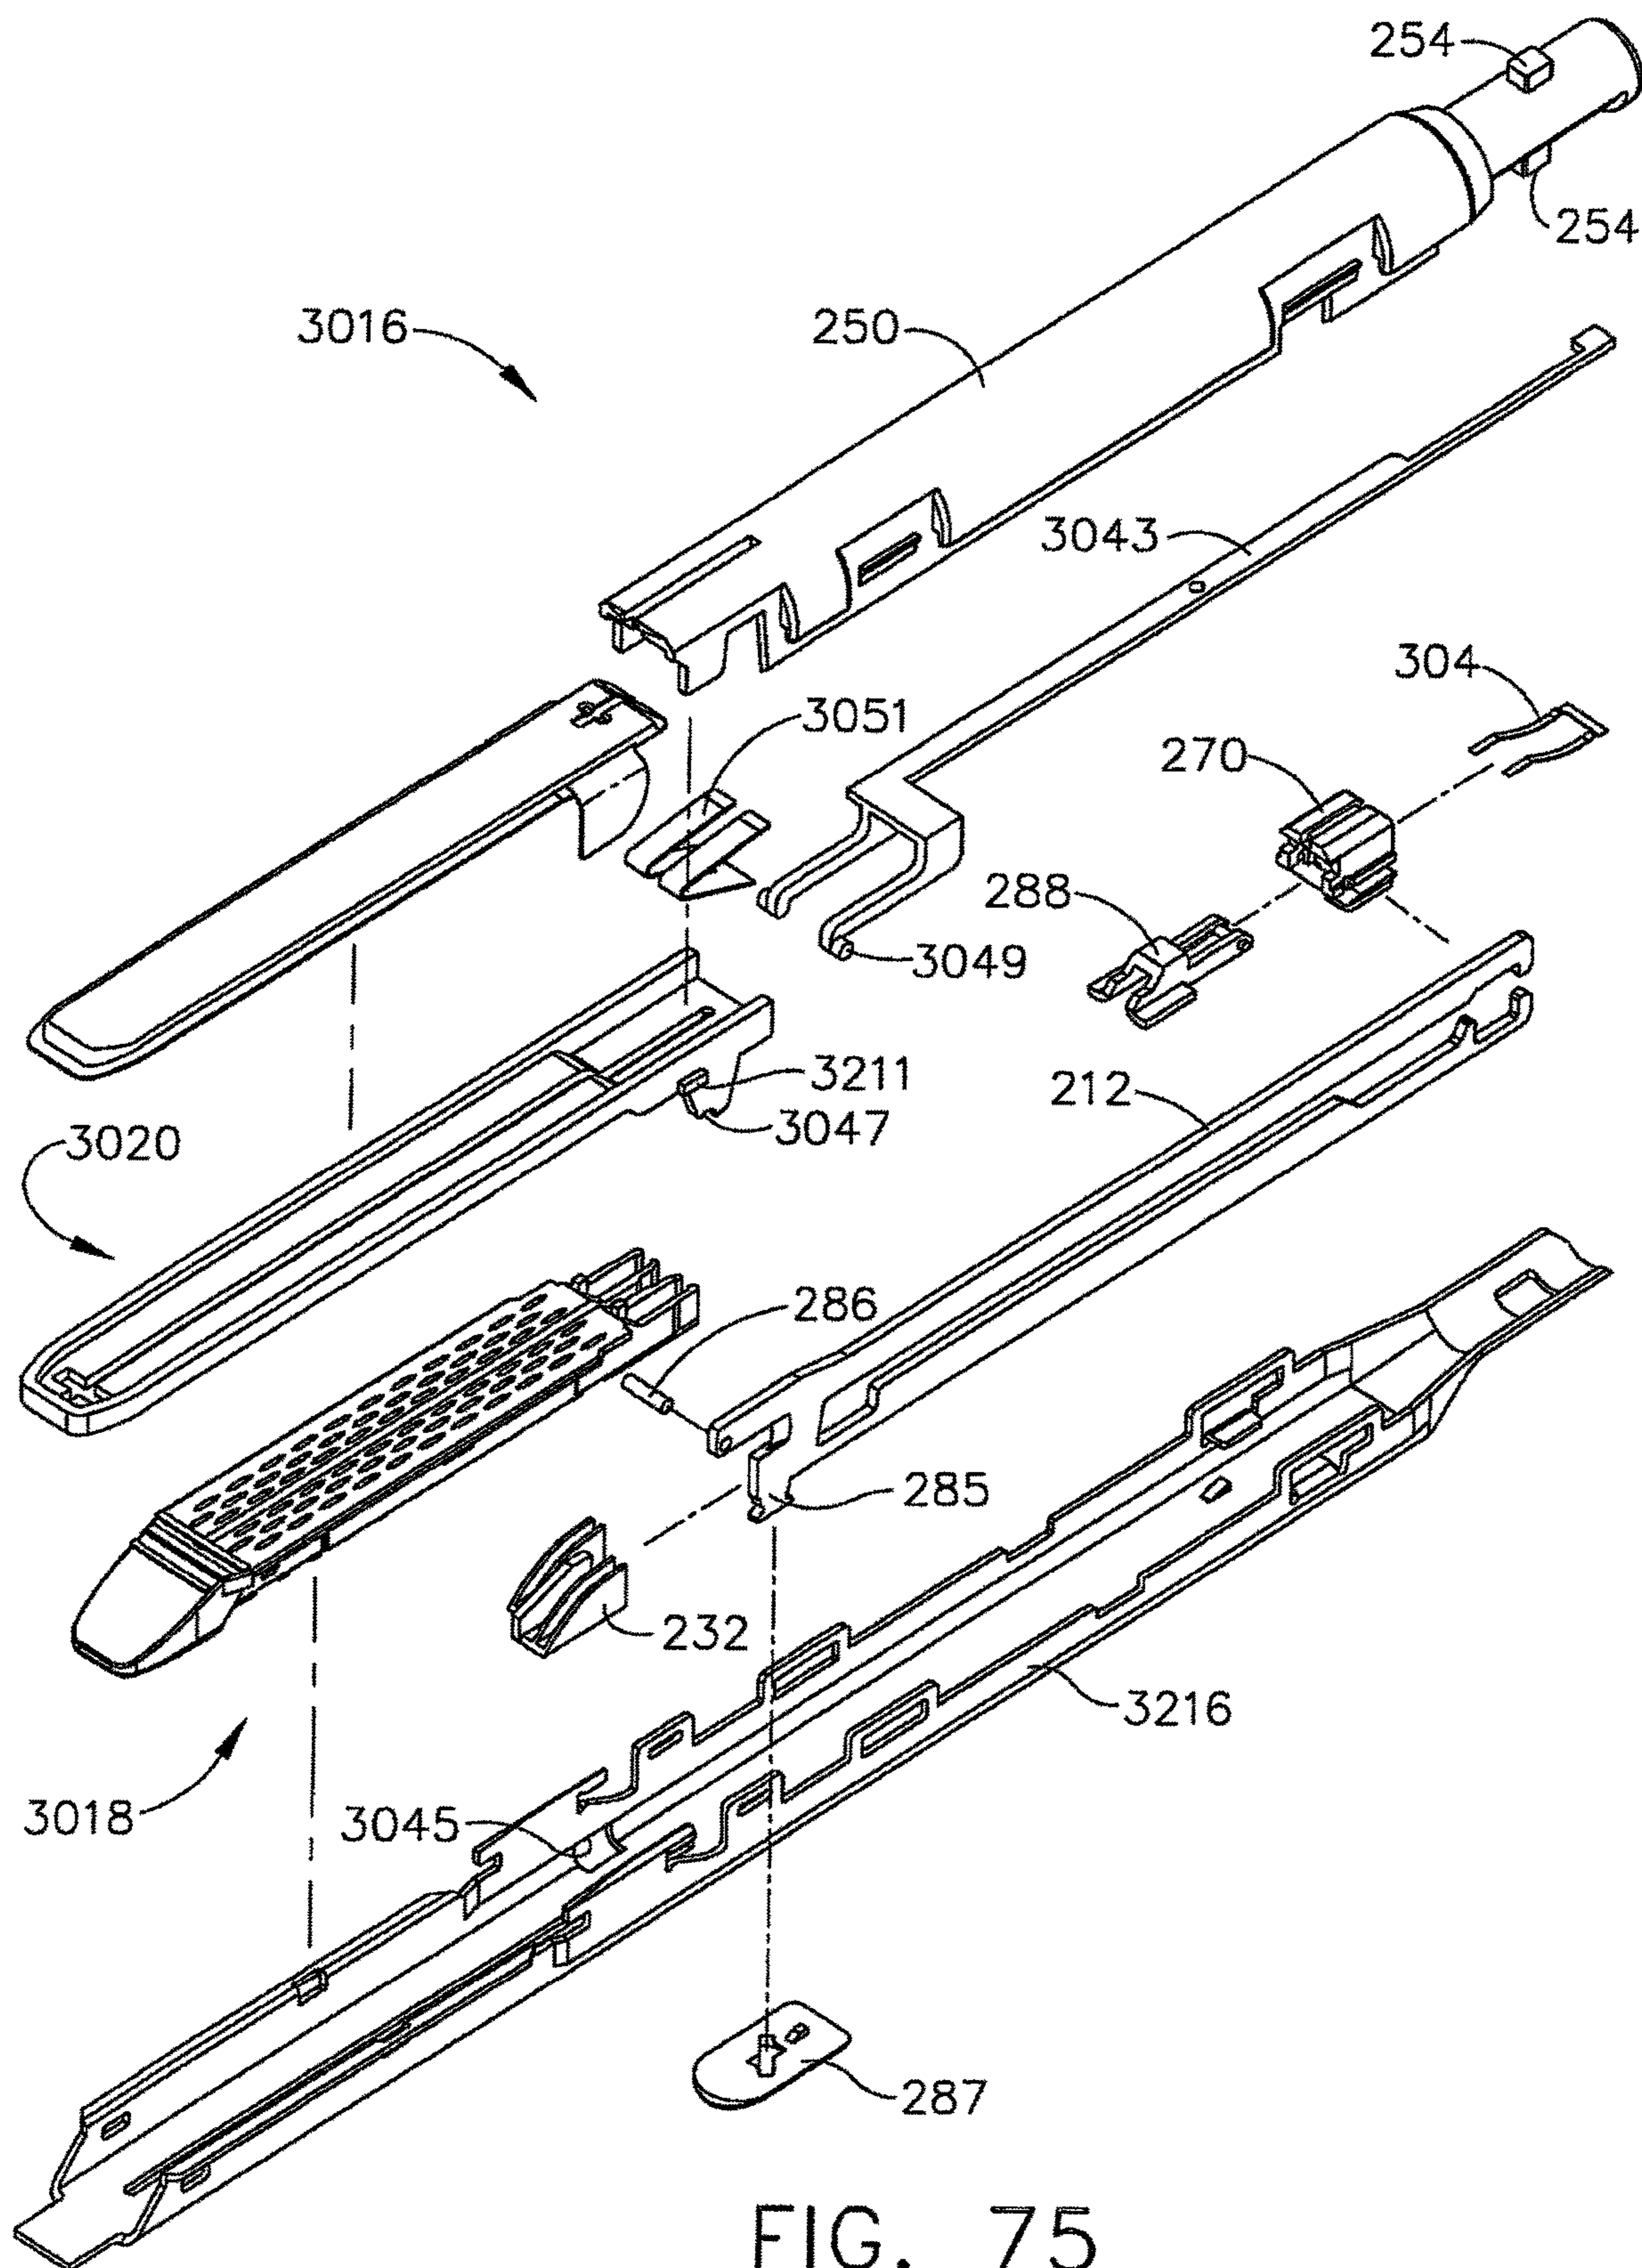
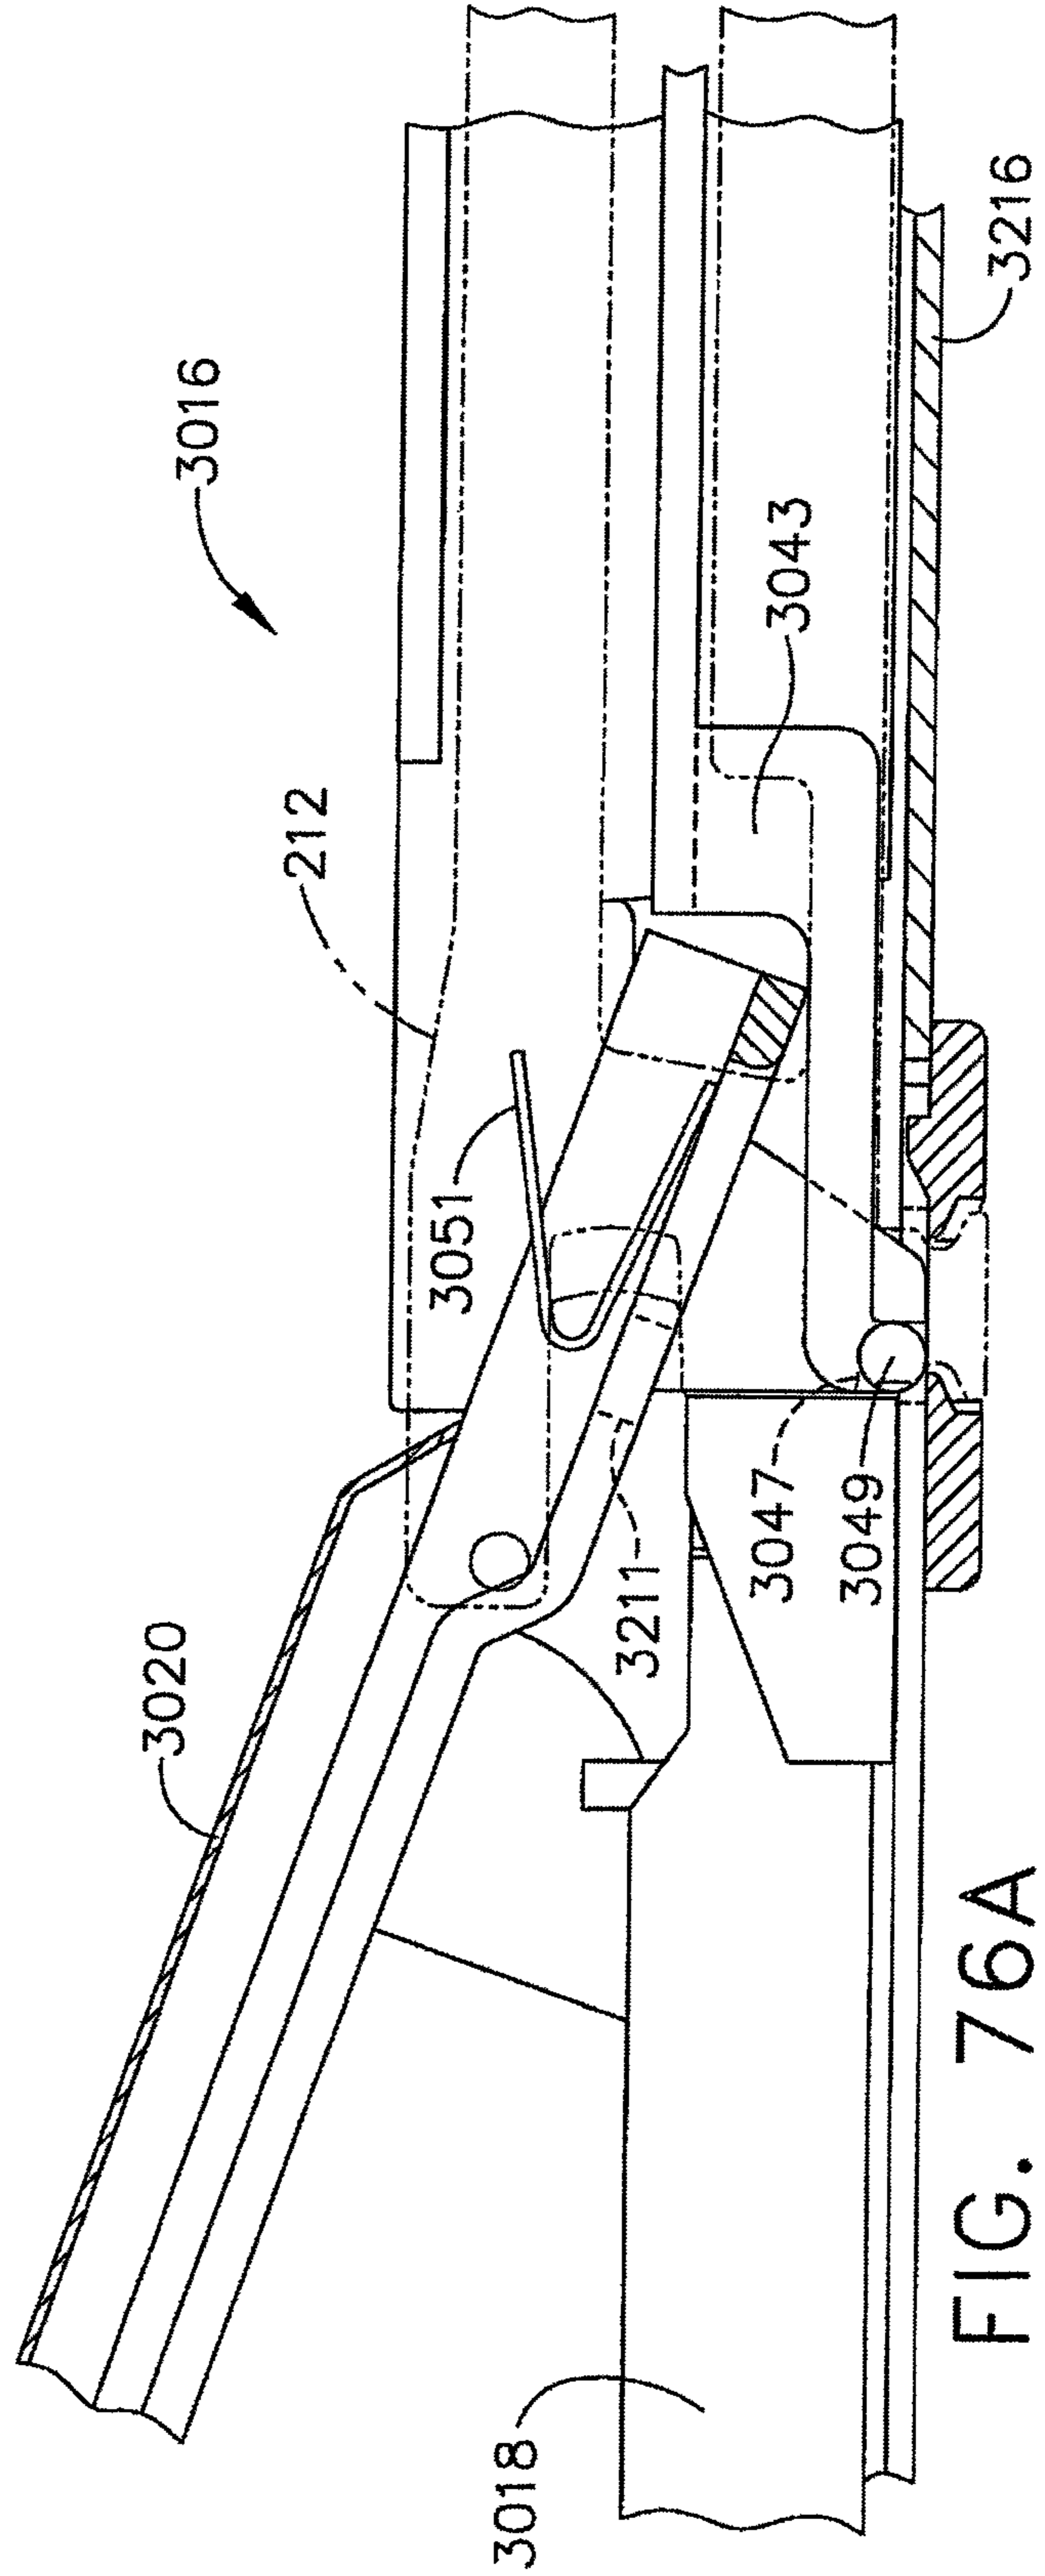
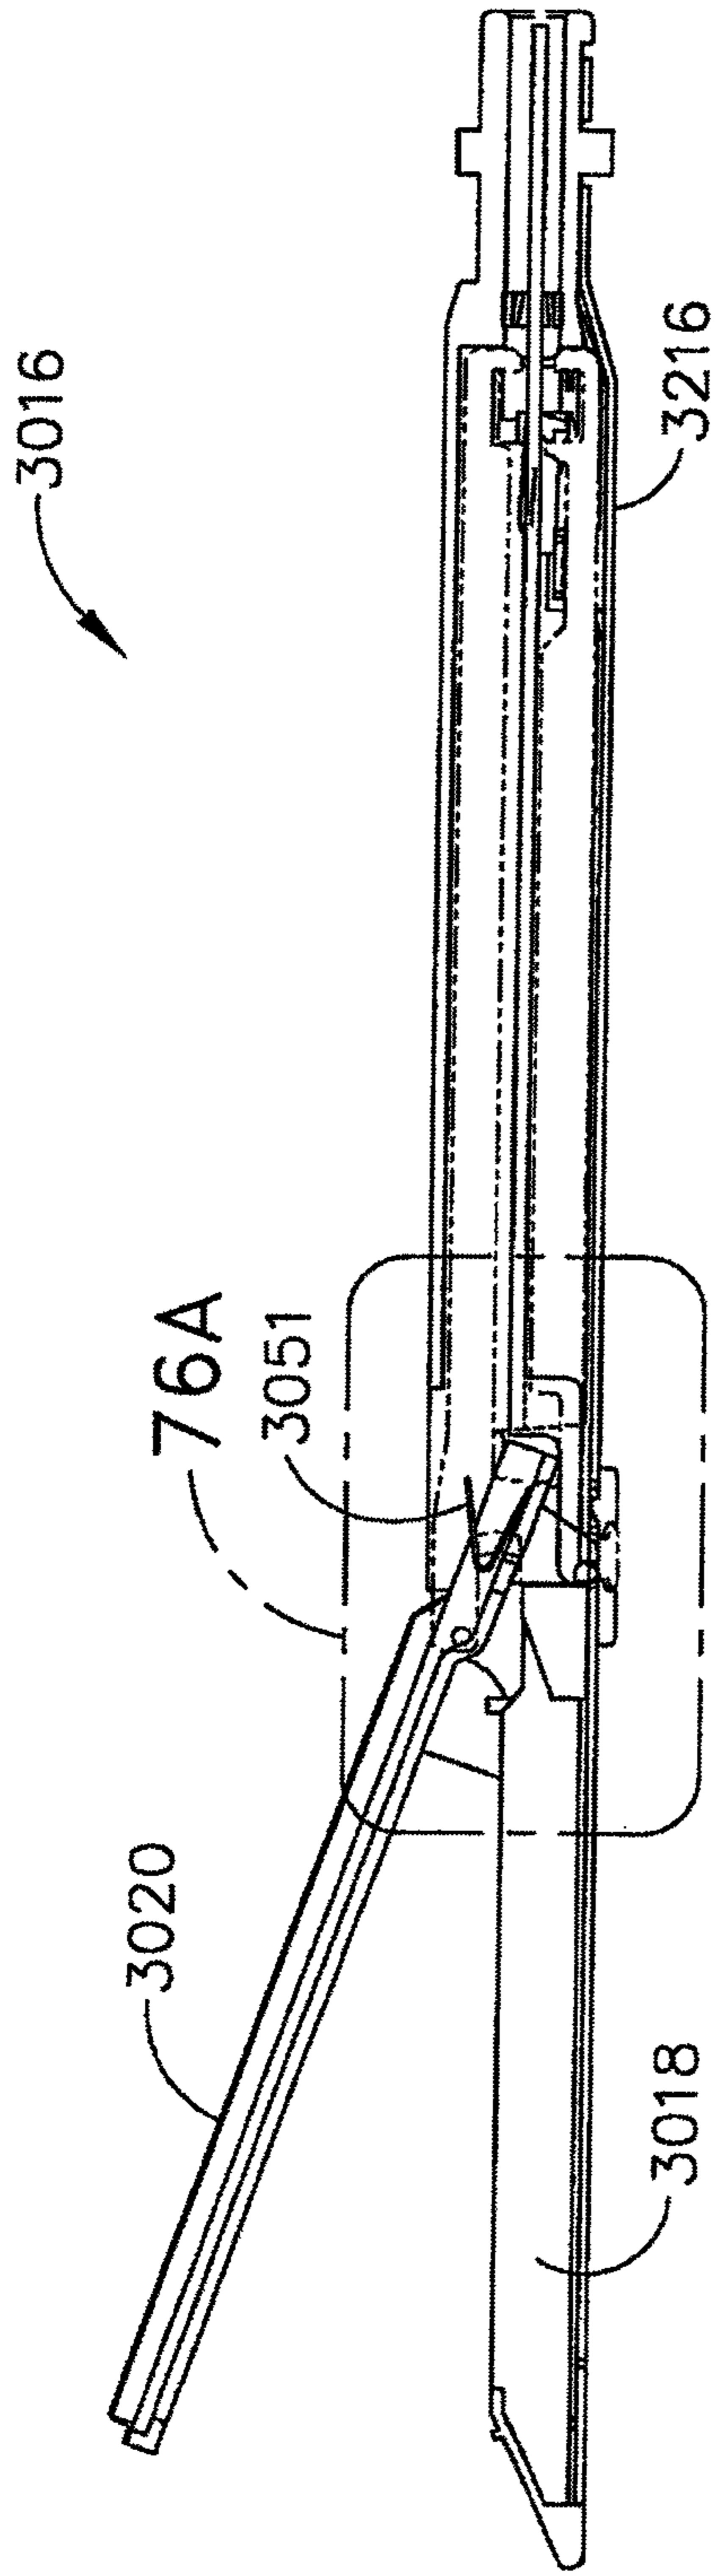


FIG. 75





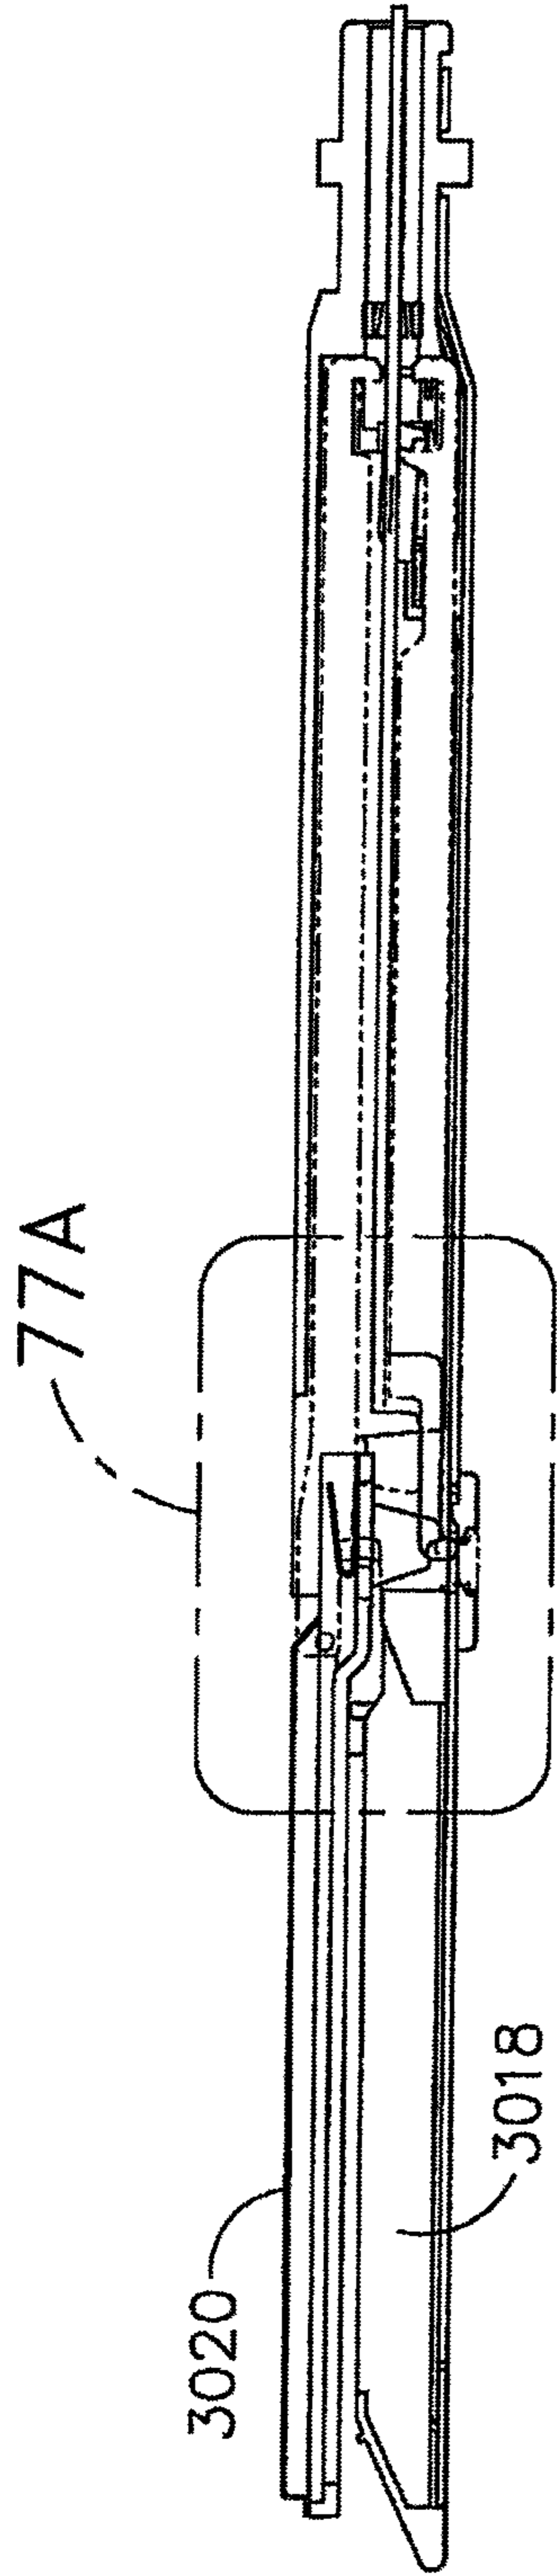


FIG. 77

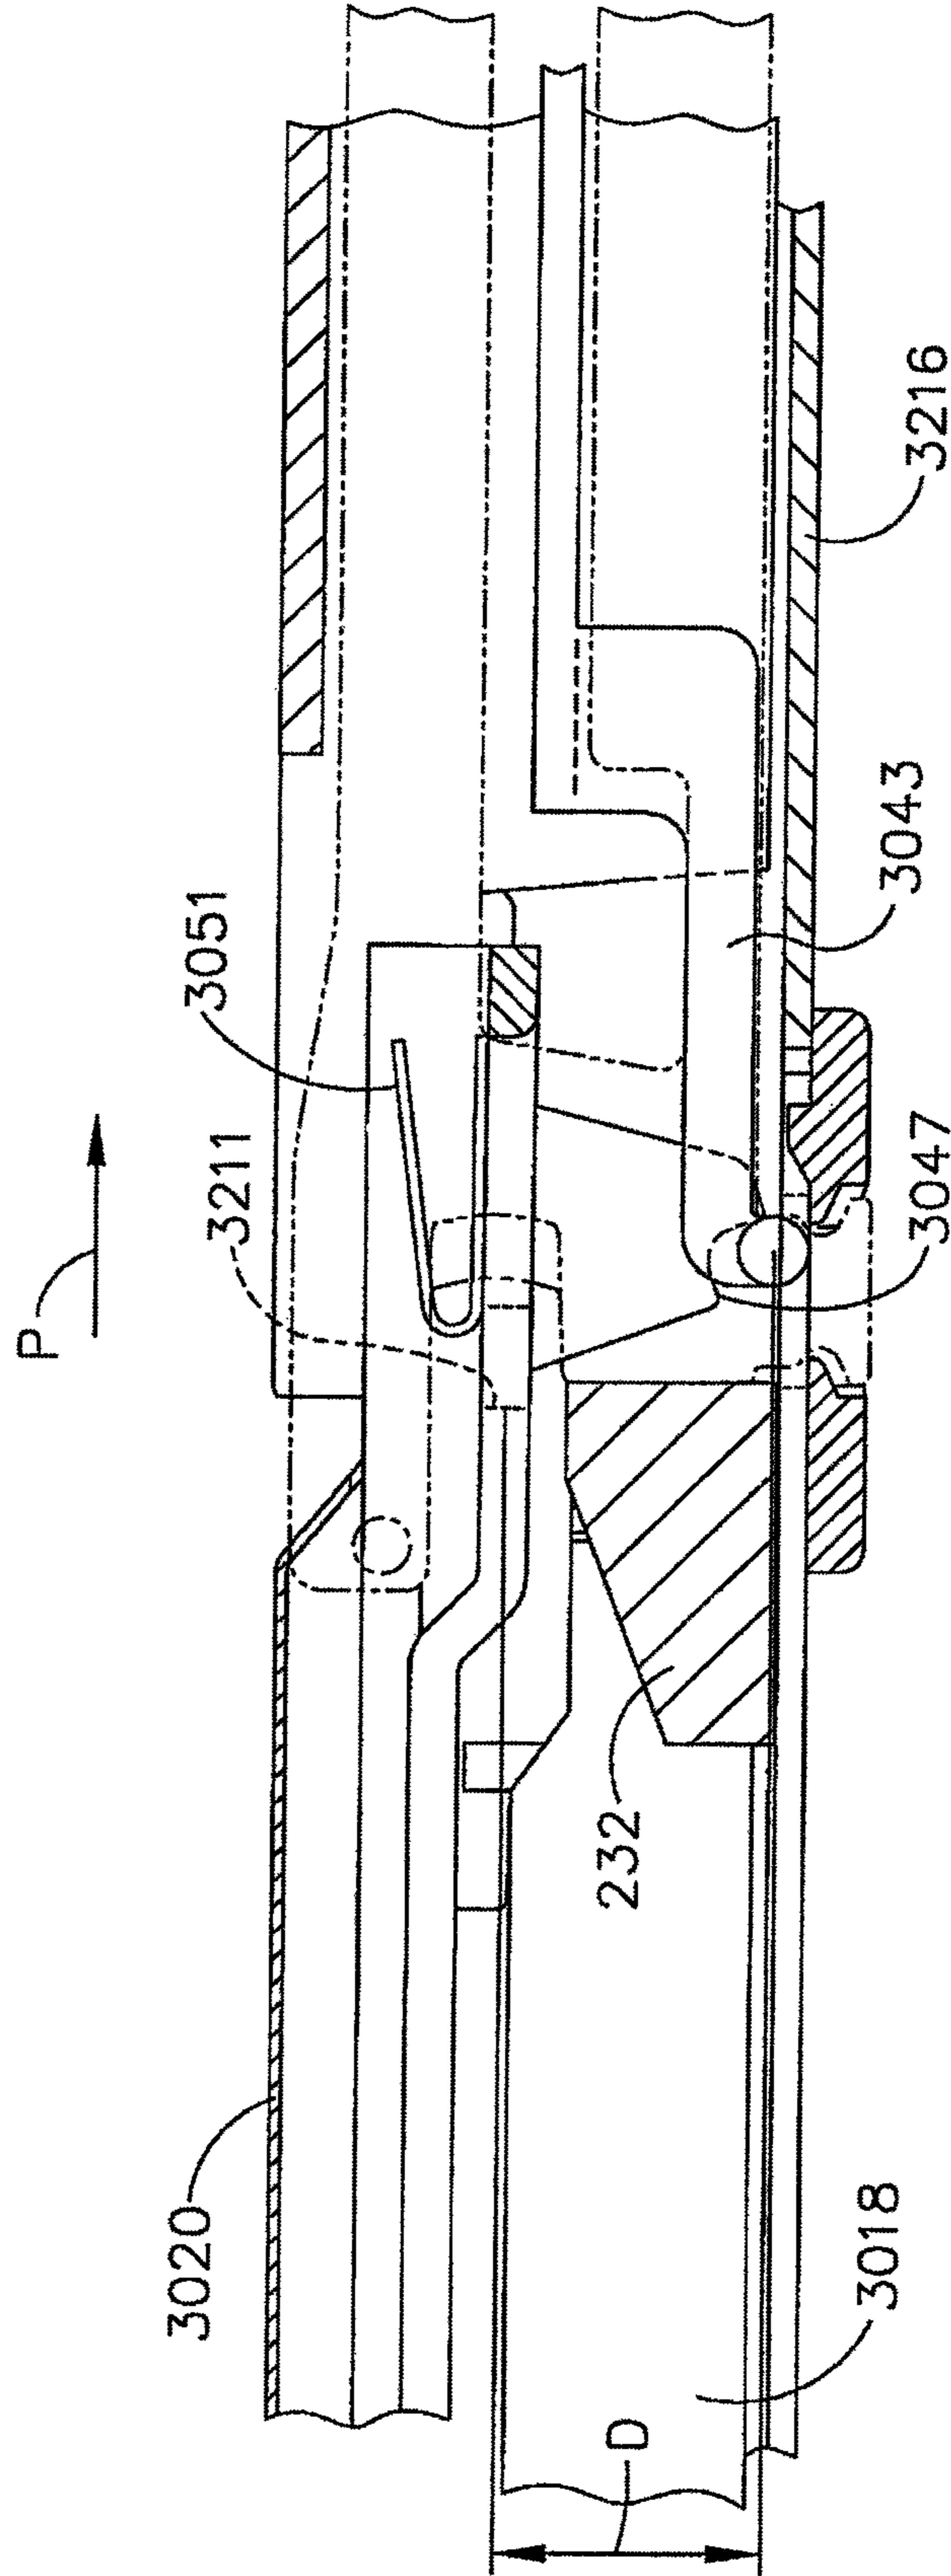


FIG. 77A

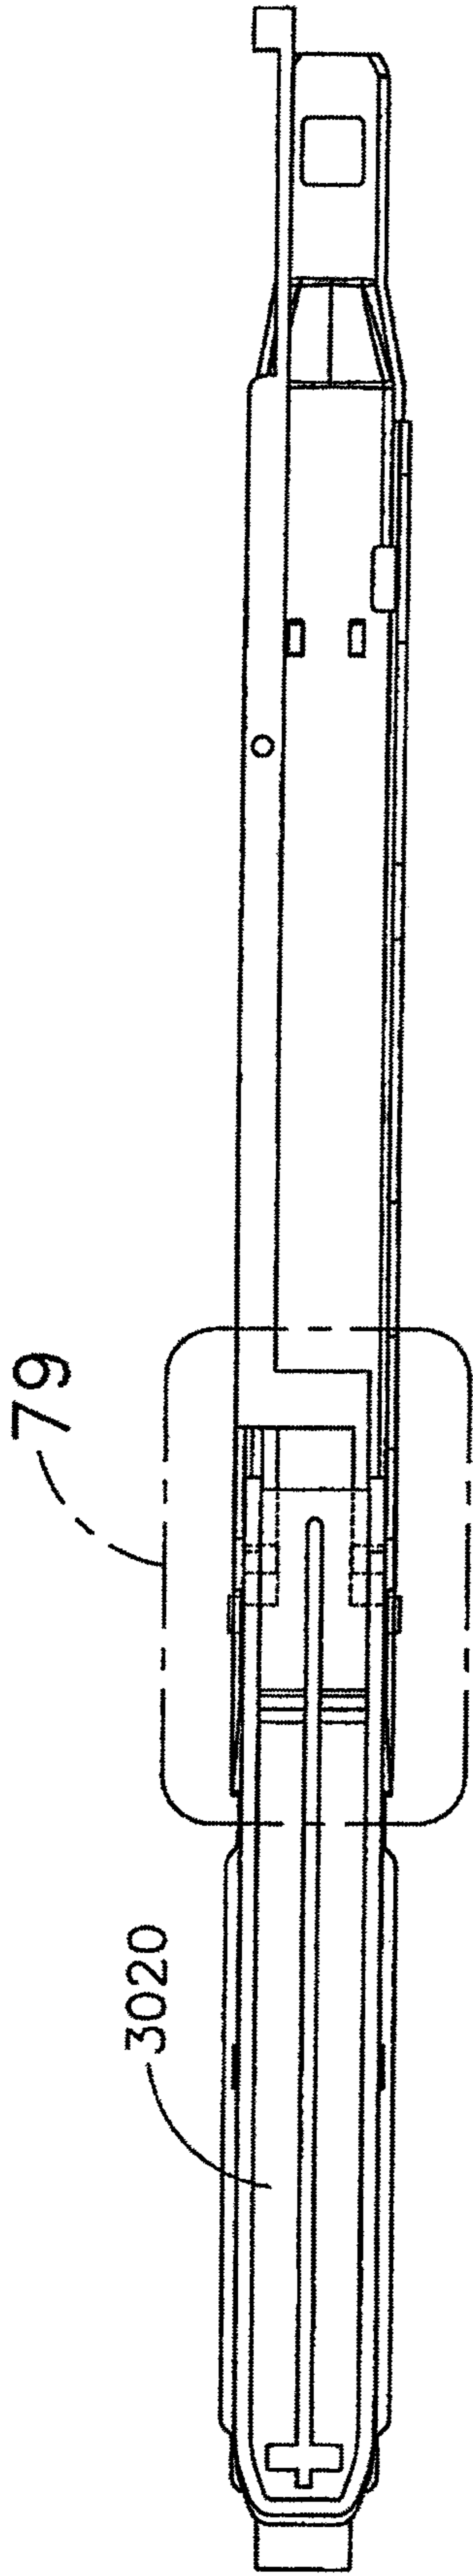


FIG. 78

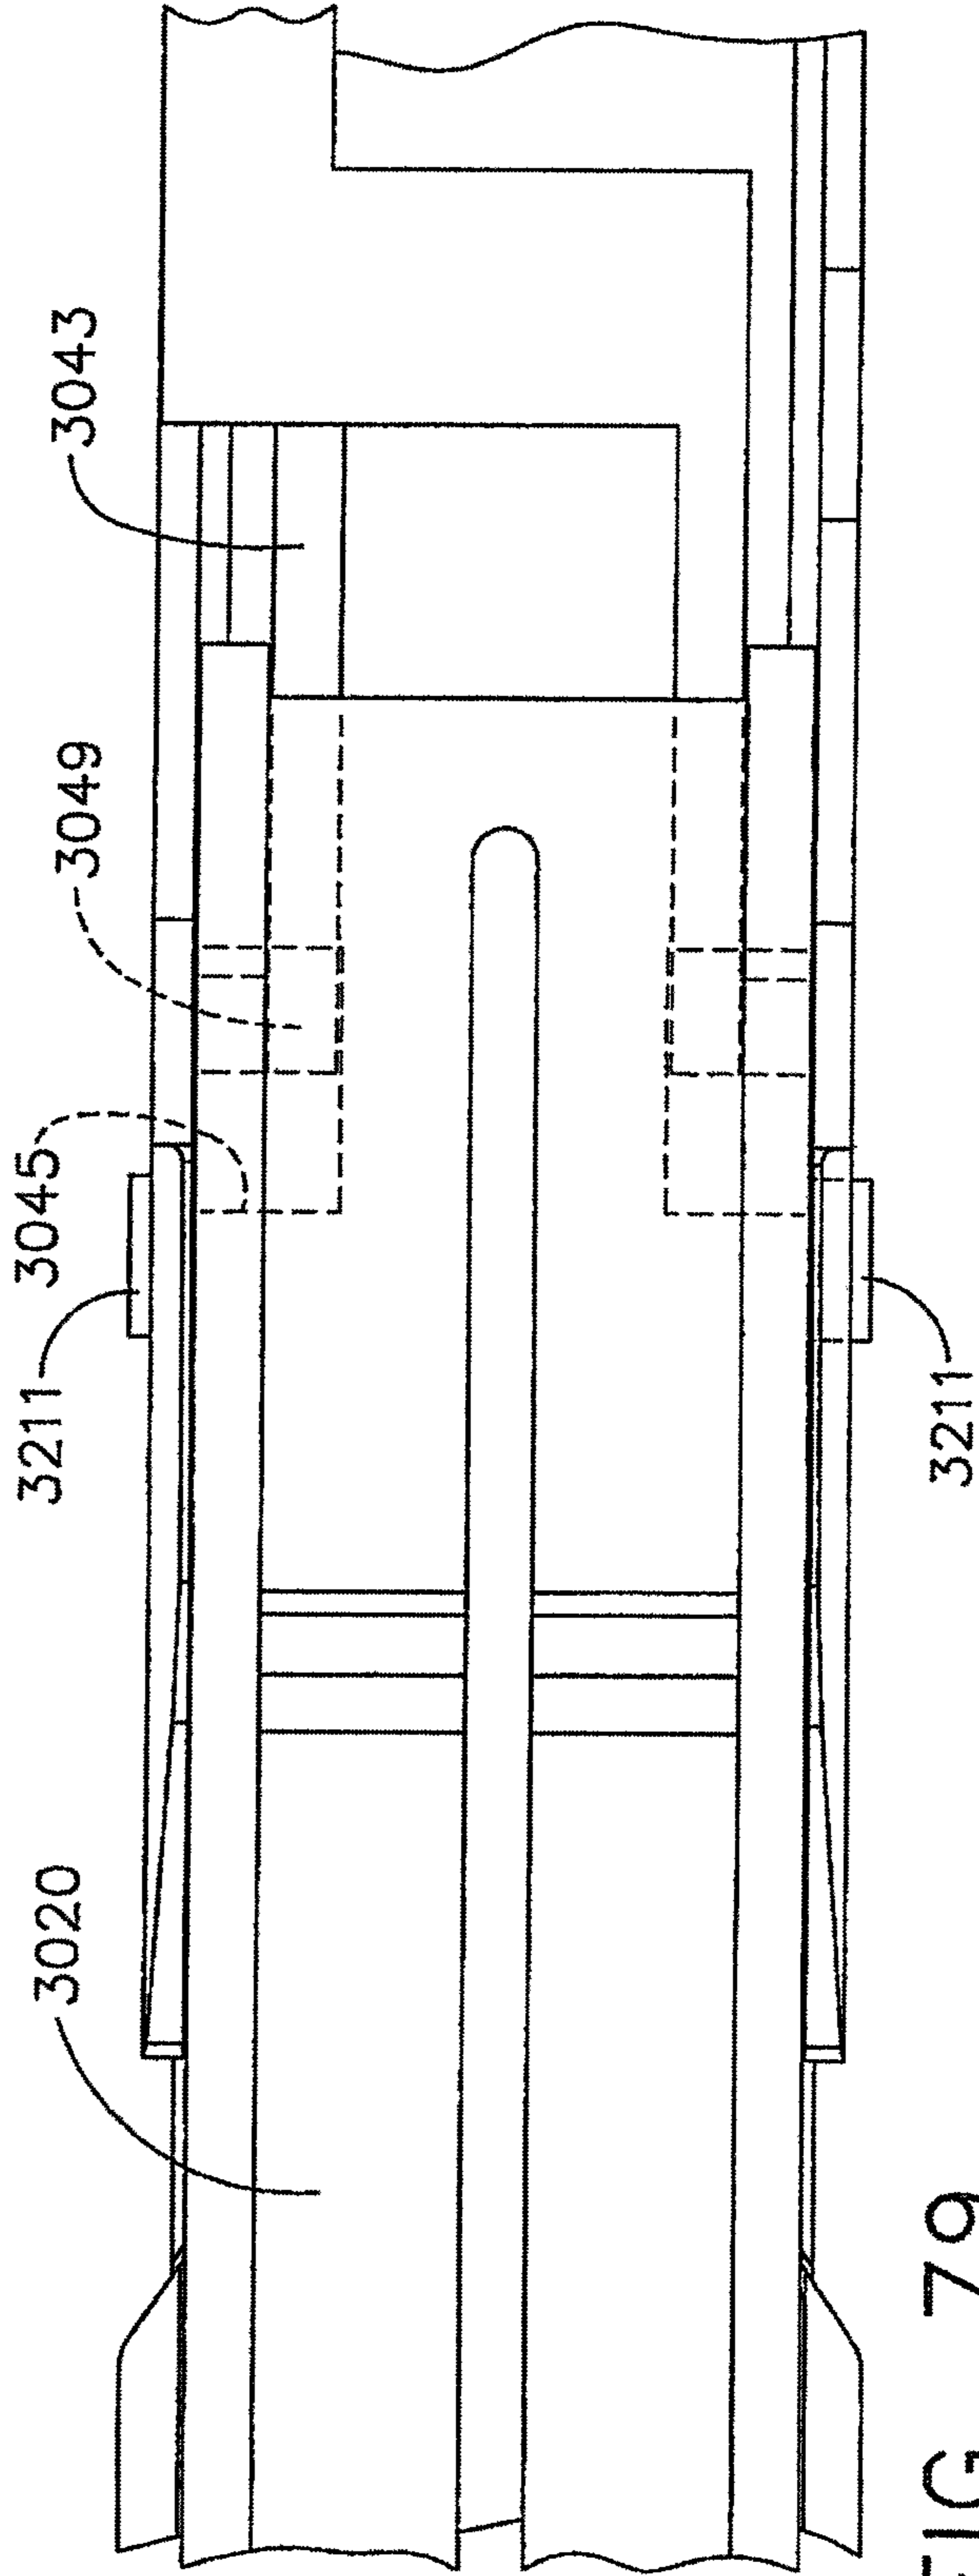


FIG. 79

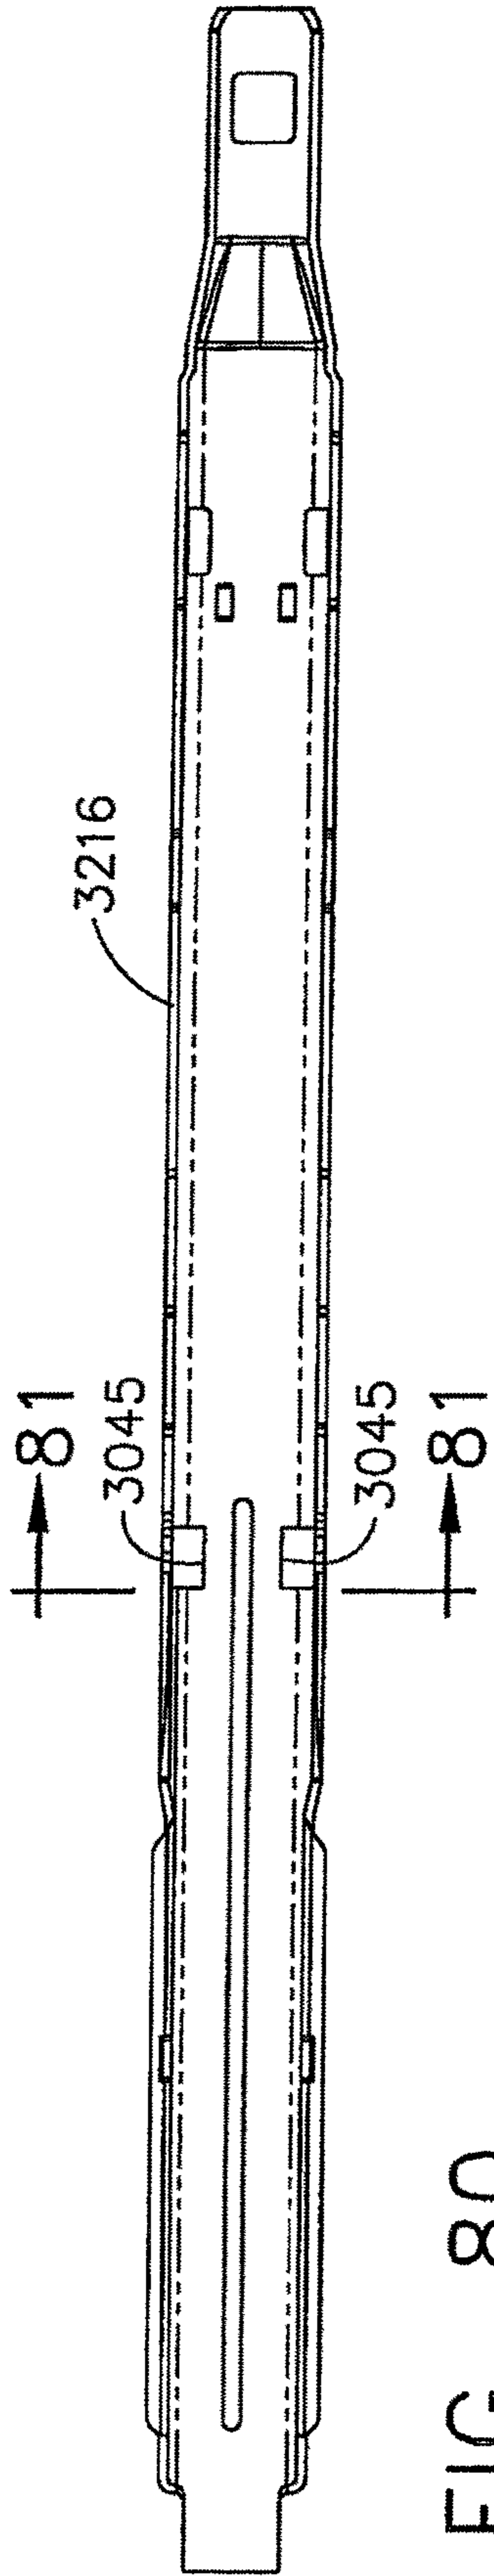


FIG. 80

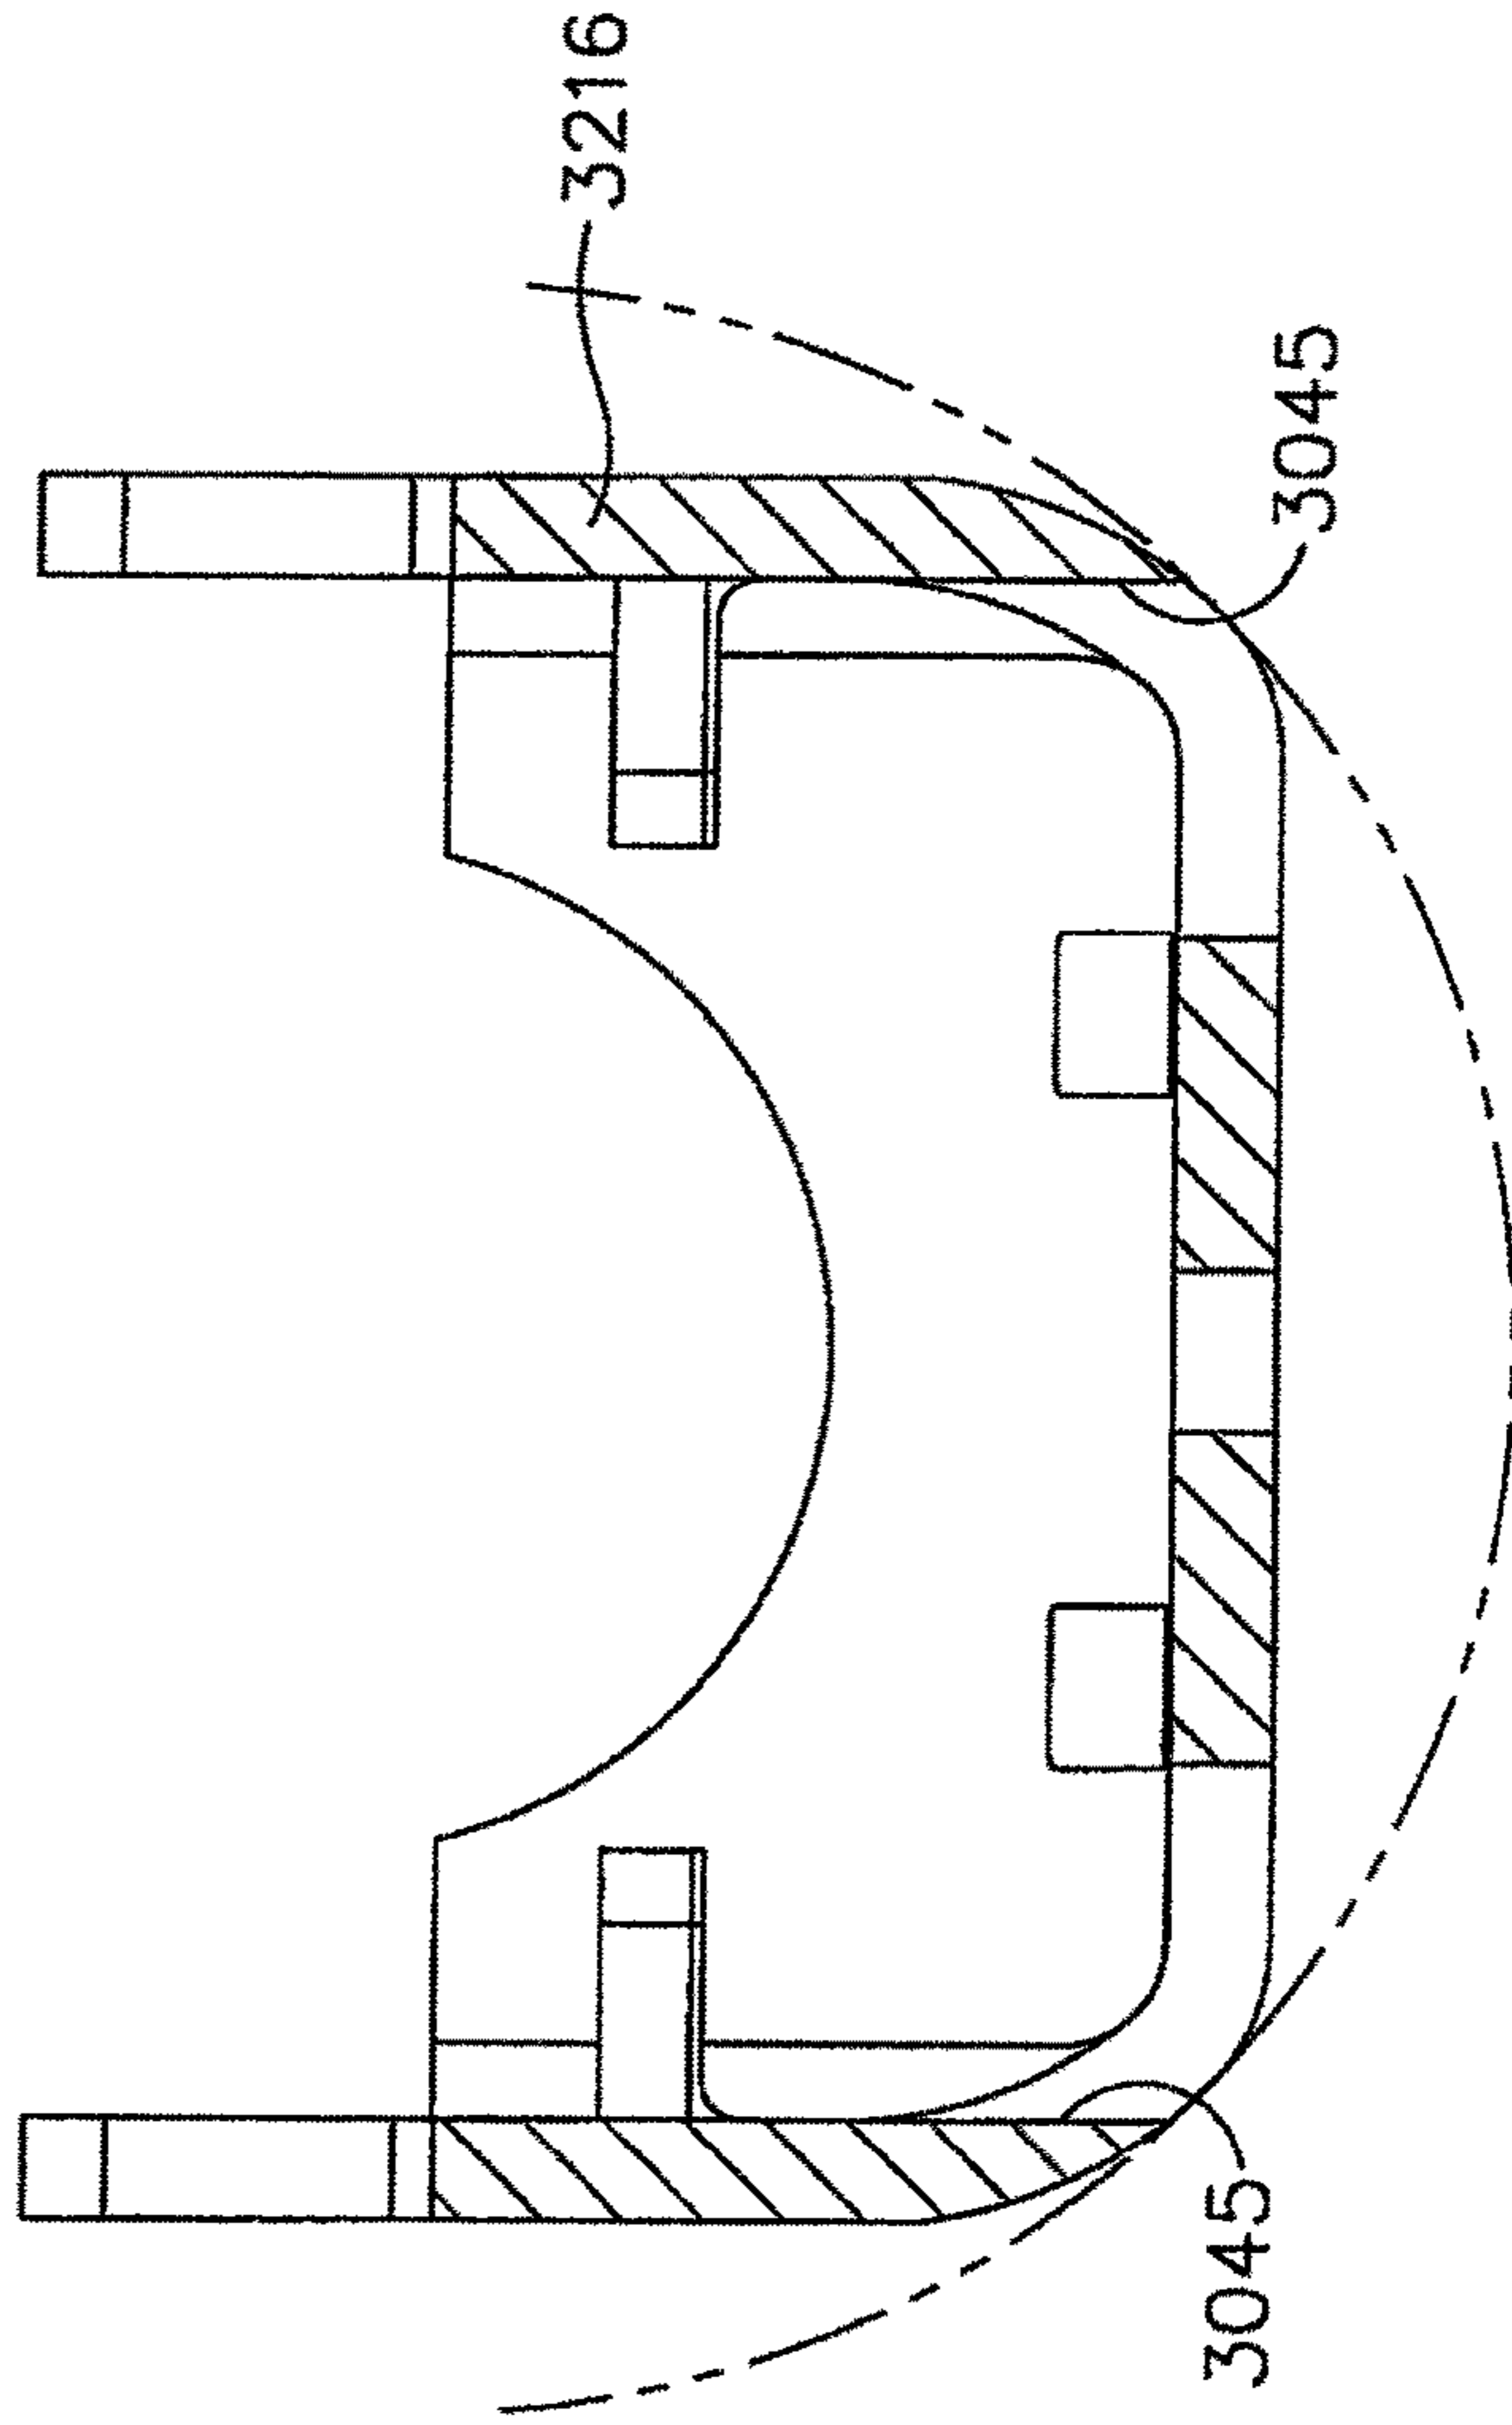


FIG. 81

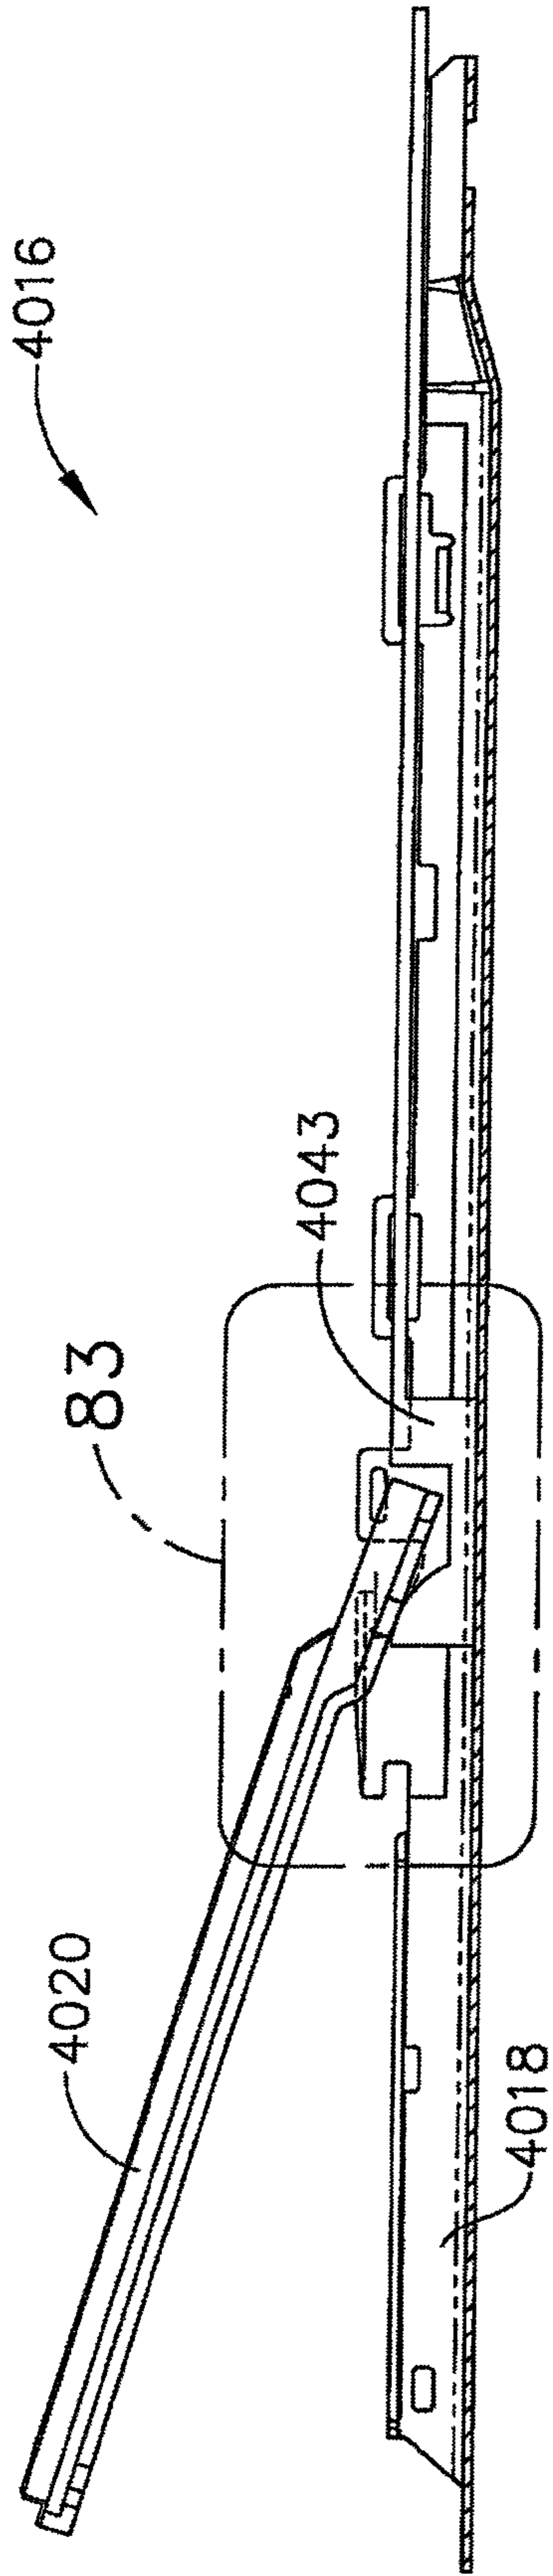


FIG. 82

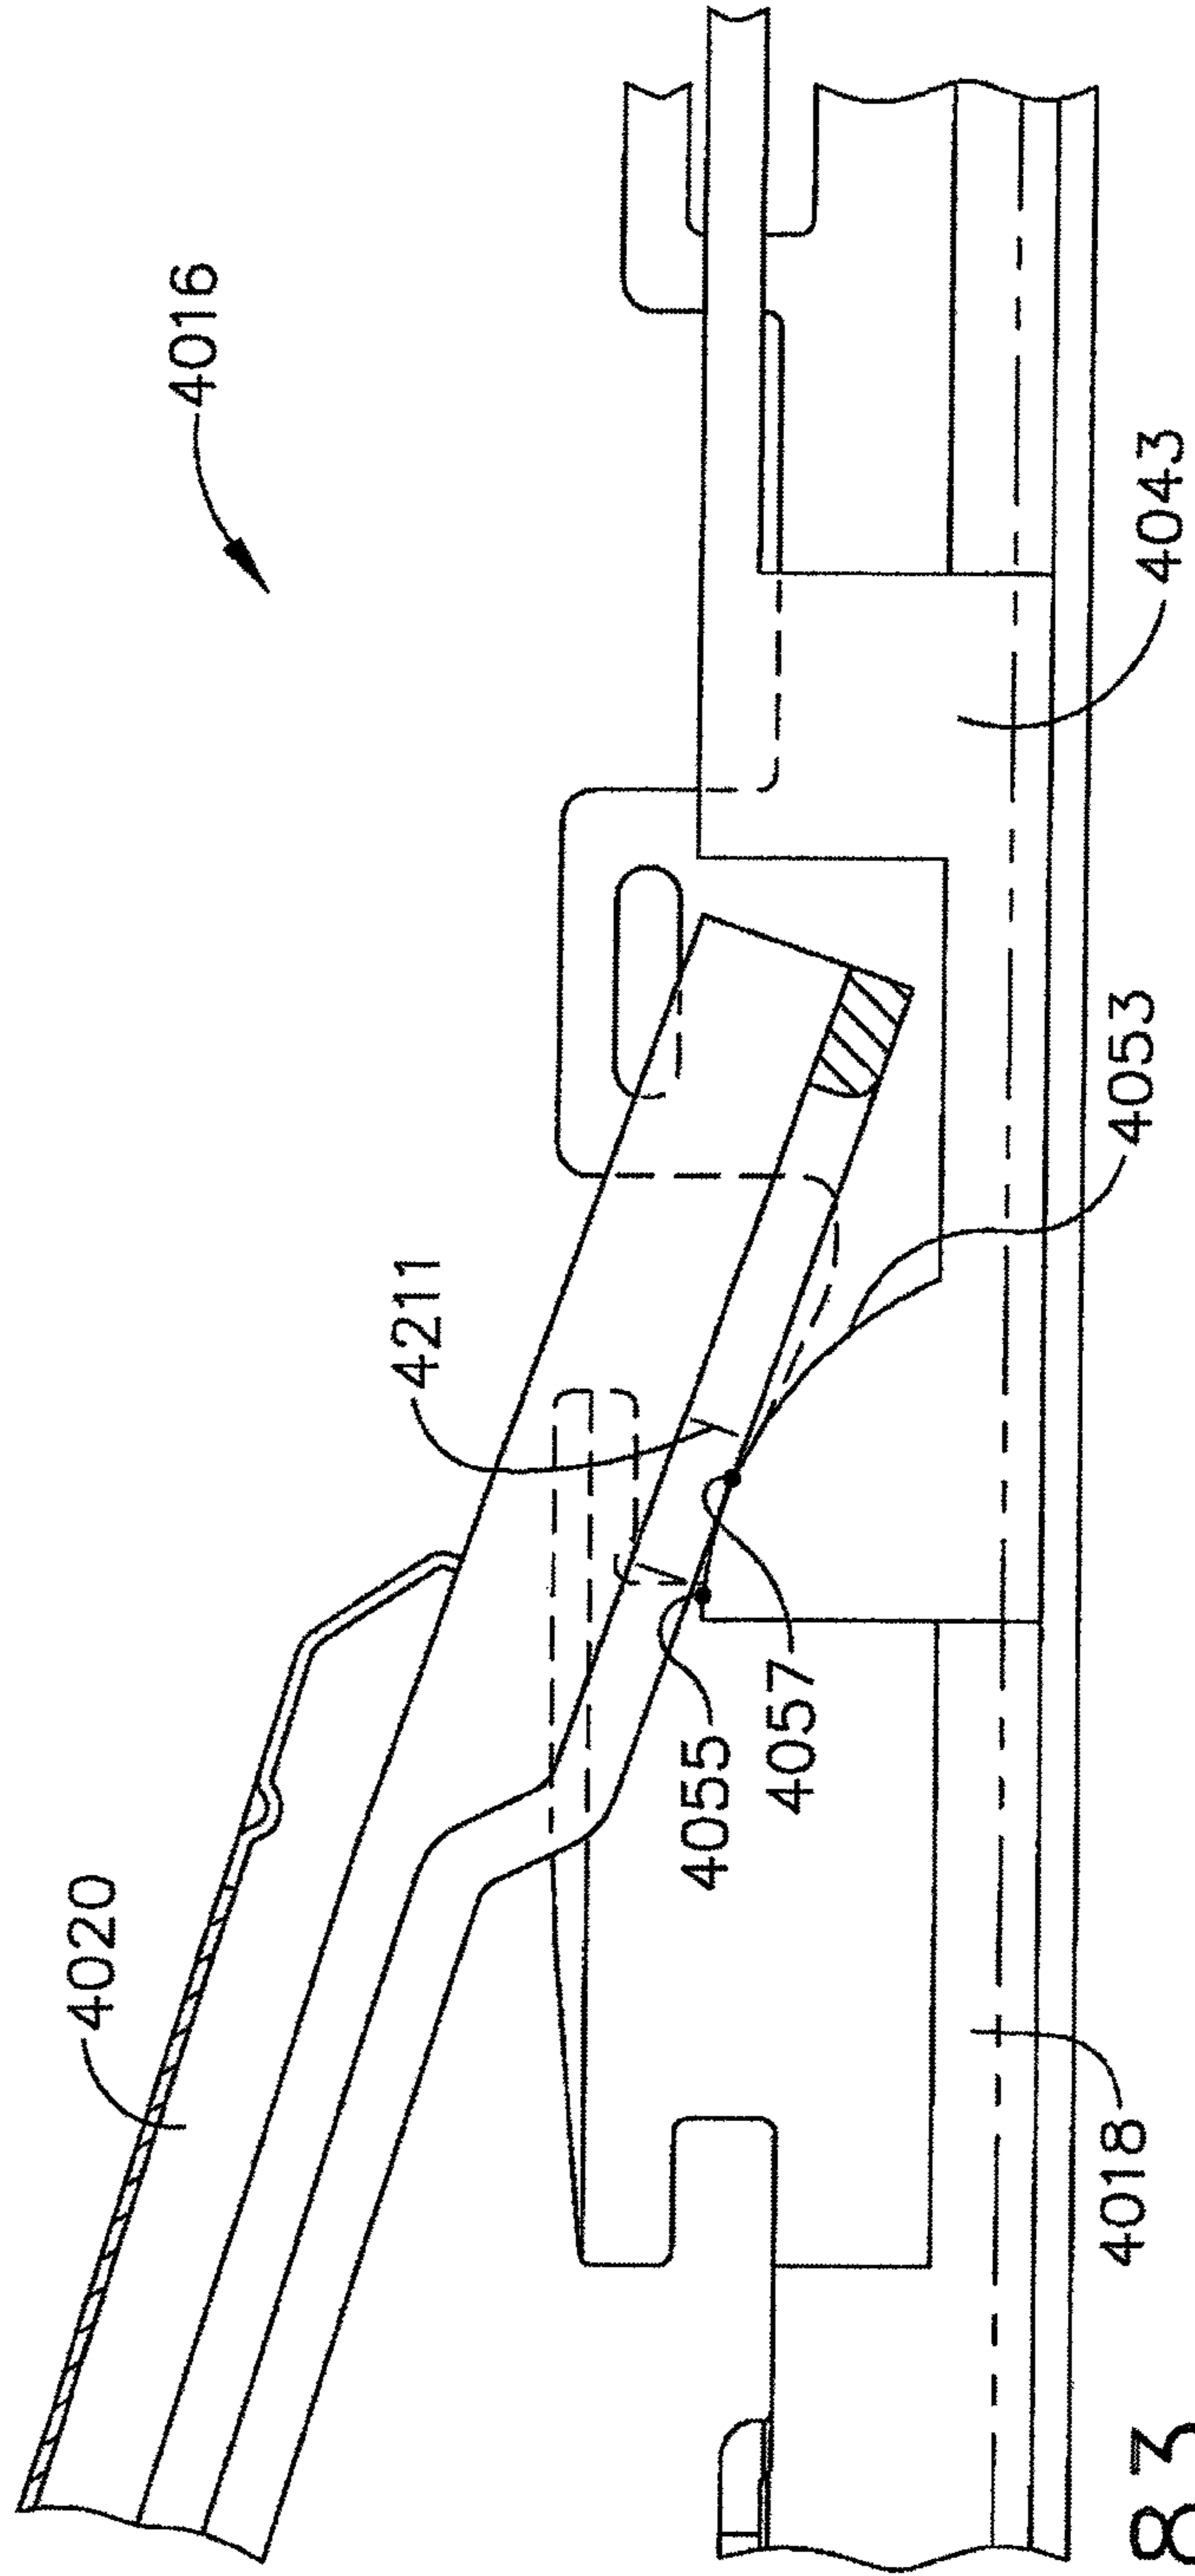


FIG. 83

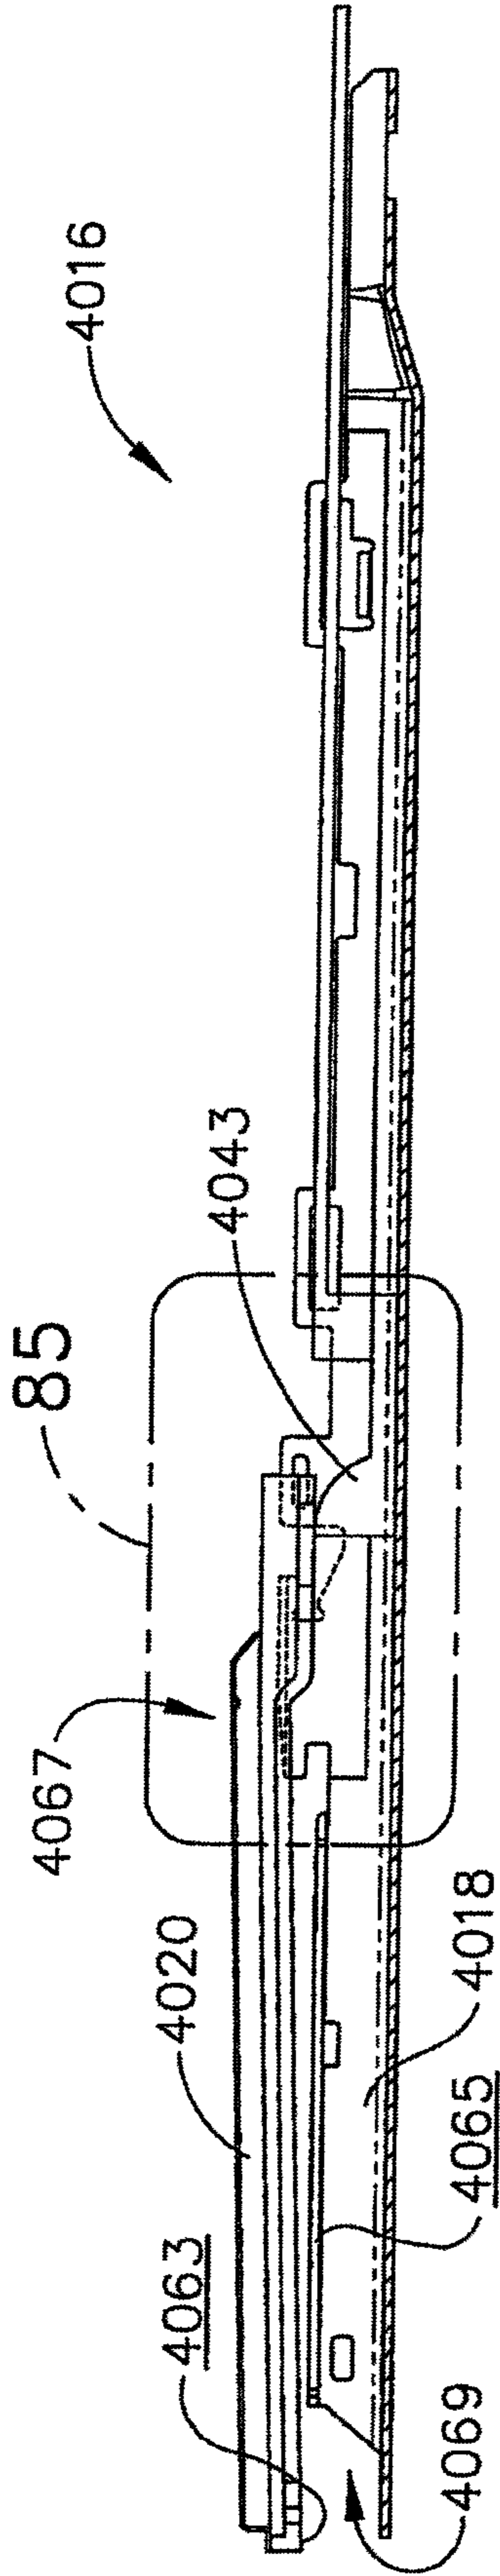


FIG. 84

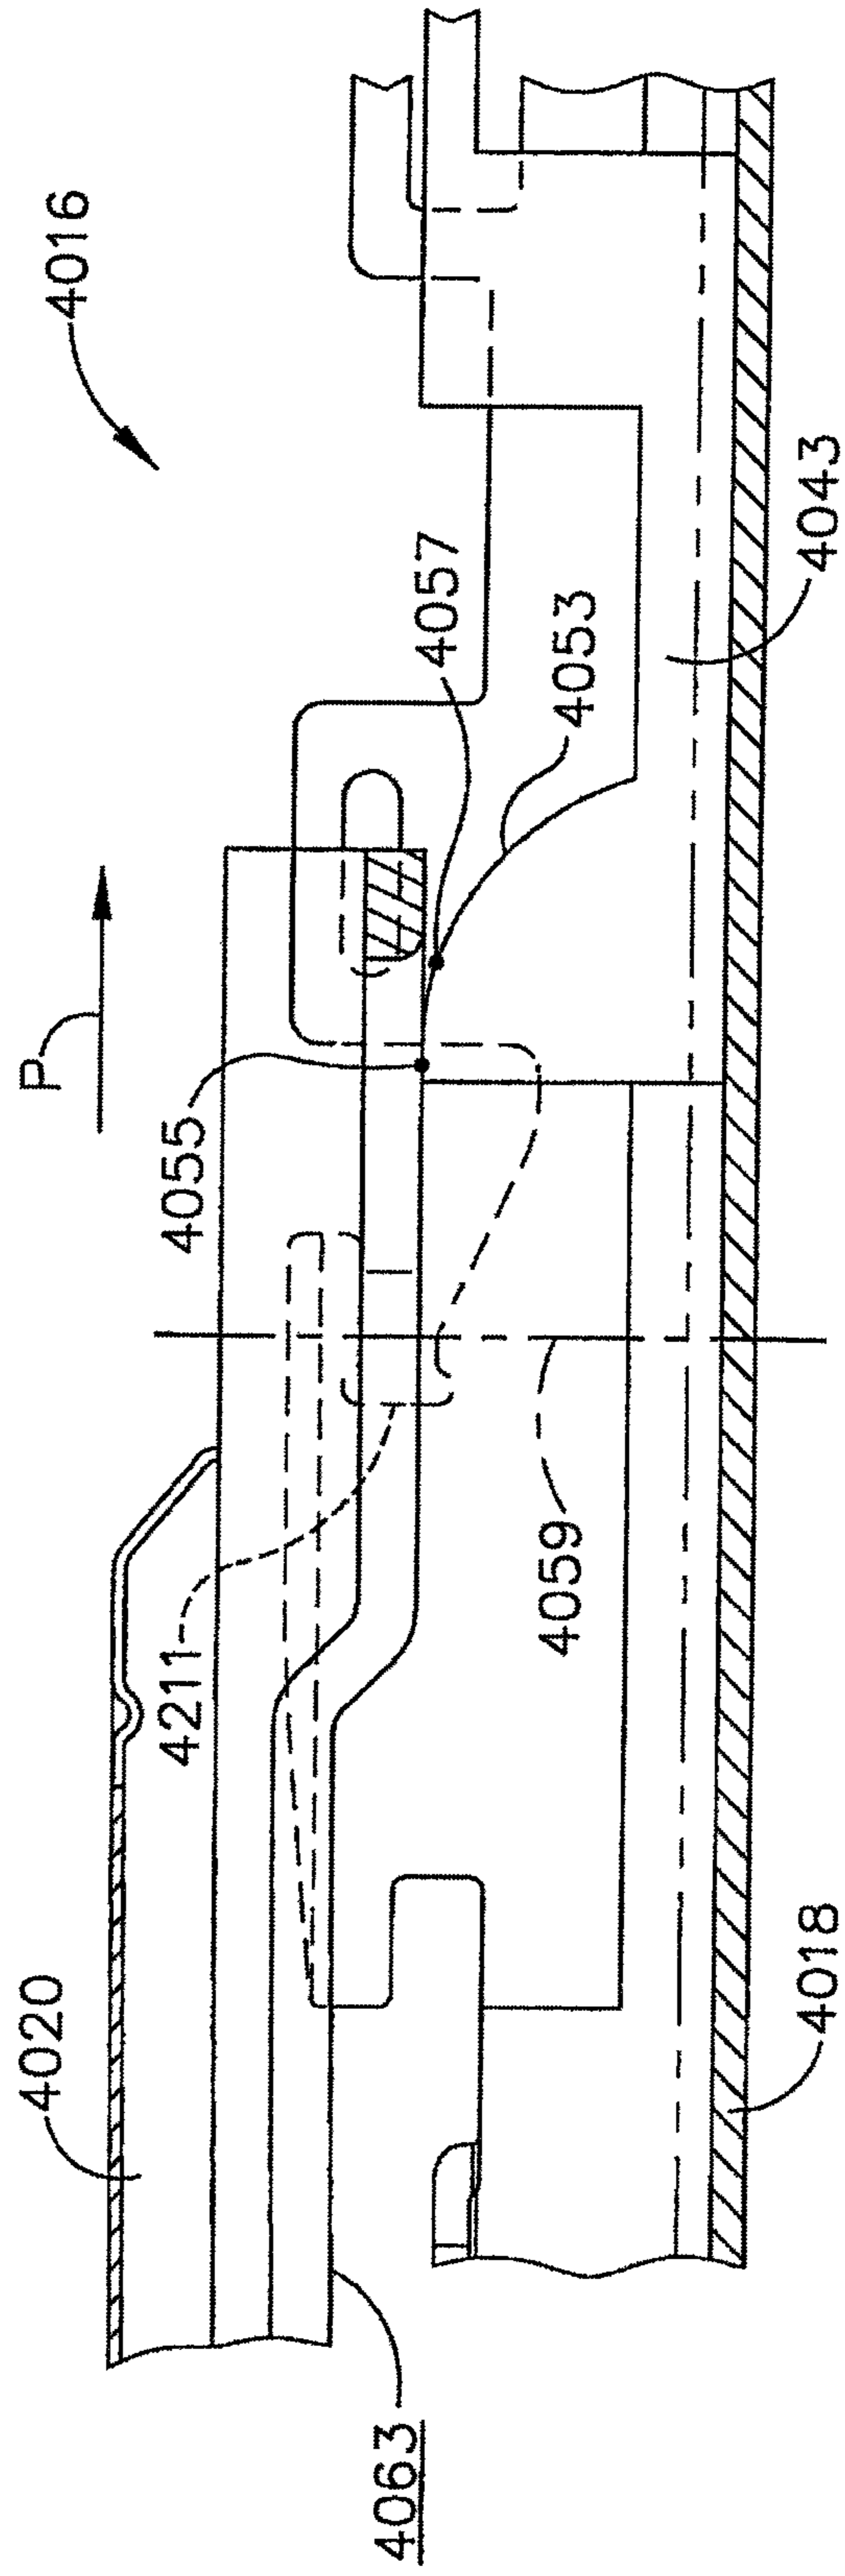


FIG. 85

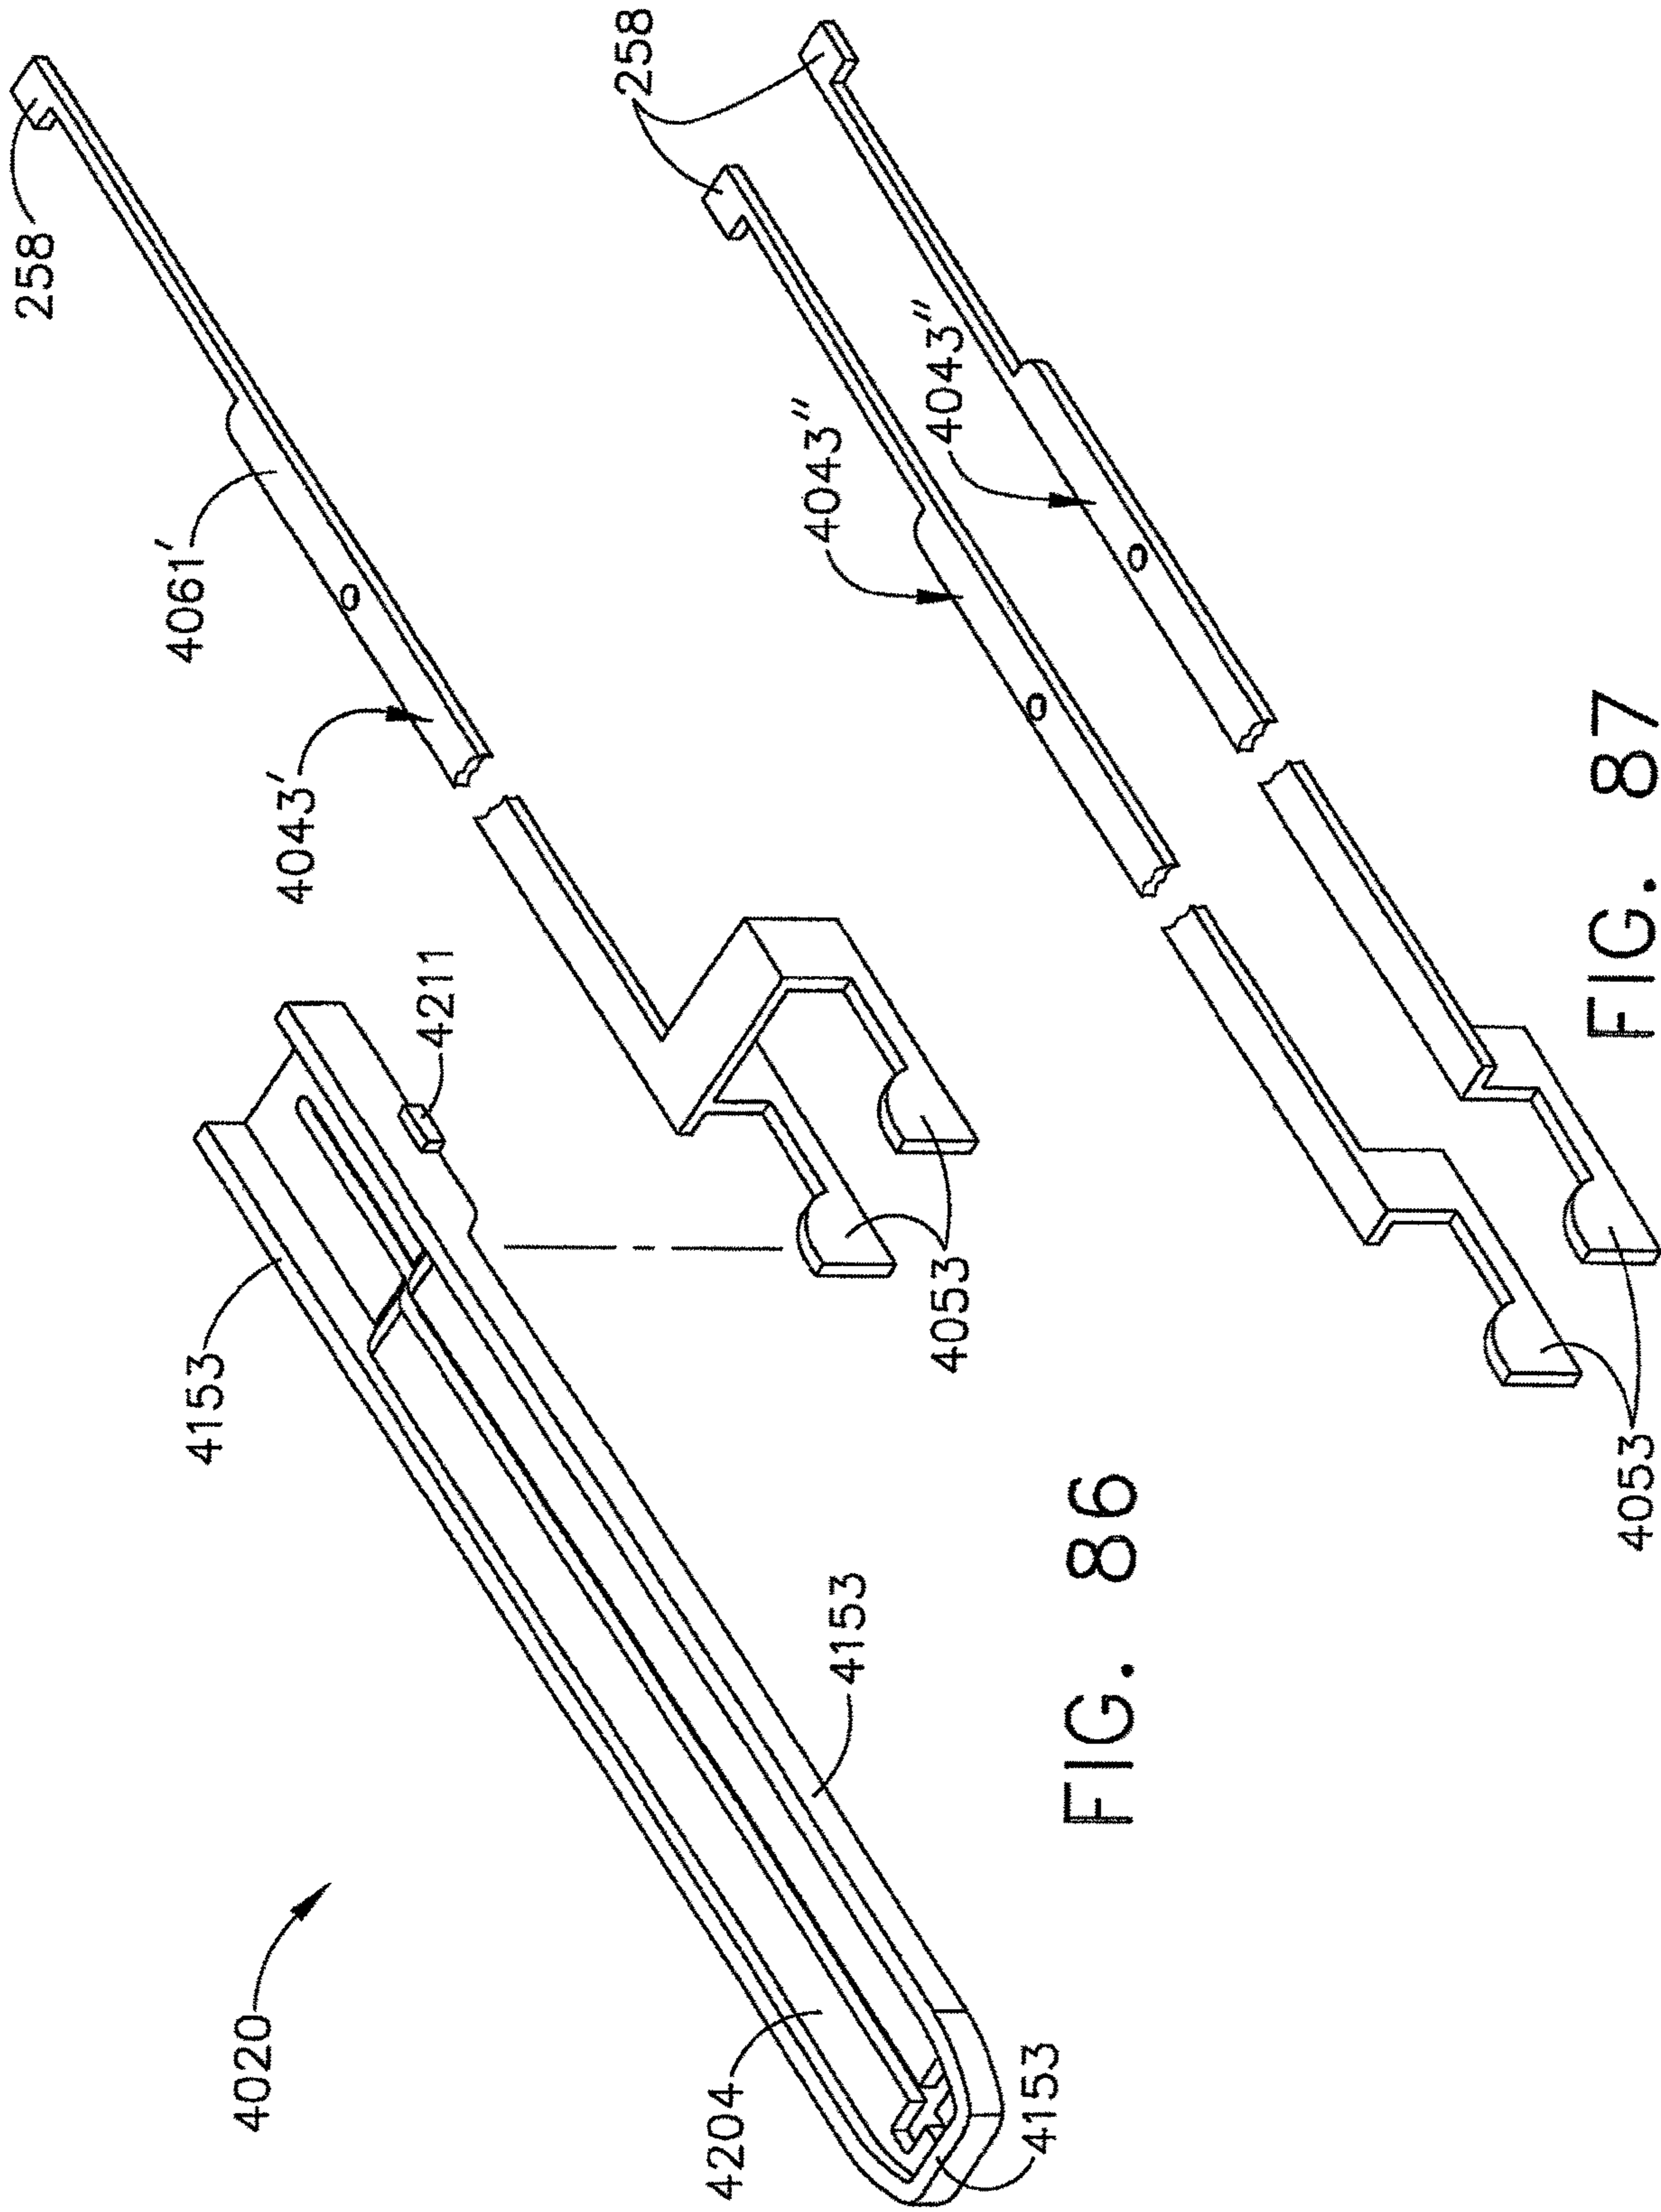


FIG. 86

FIG. 87

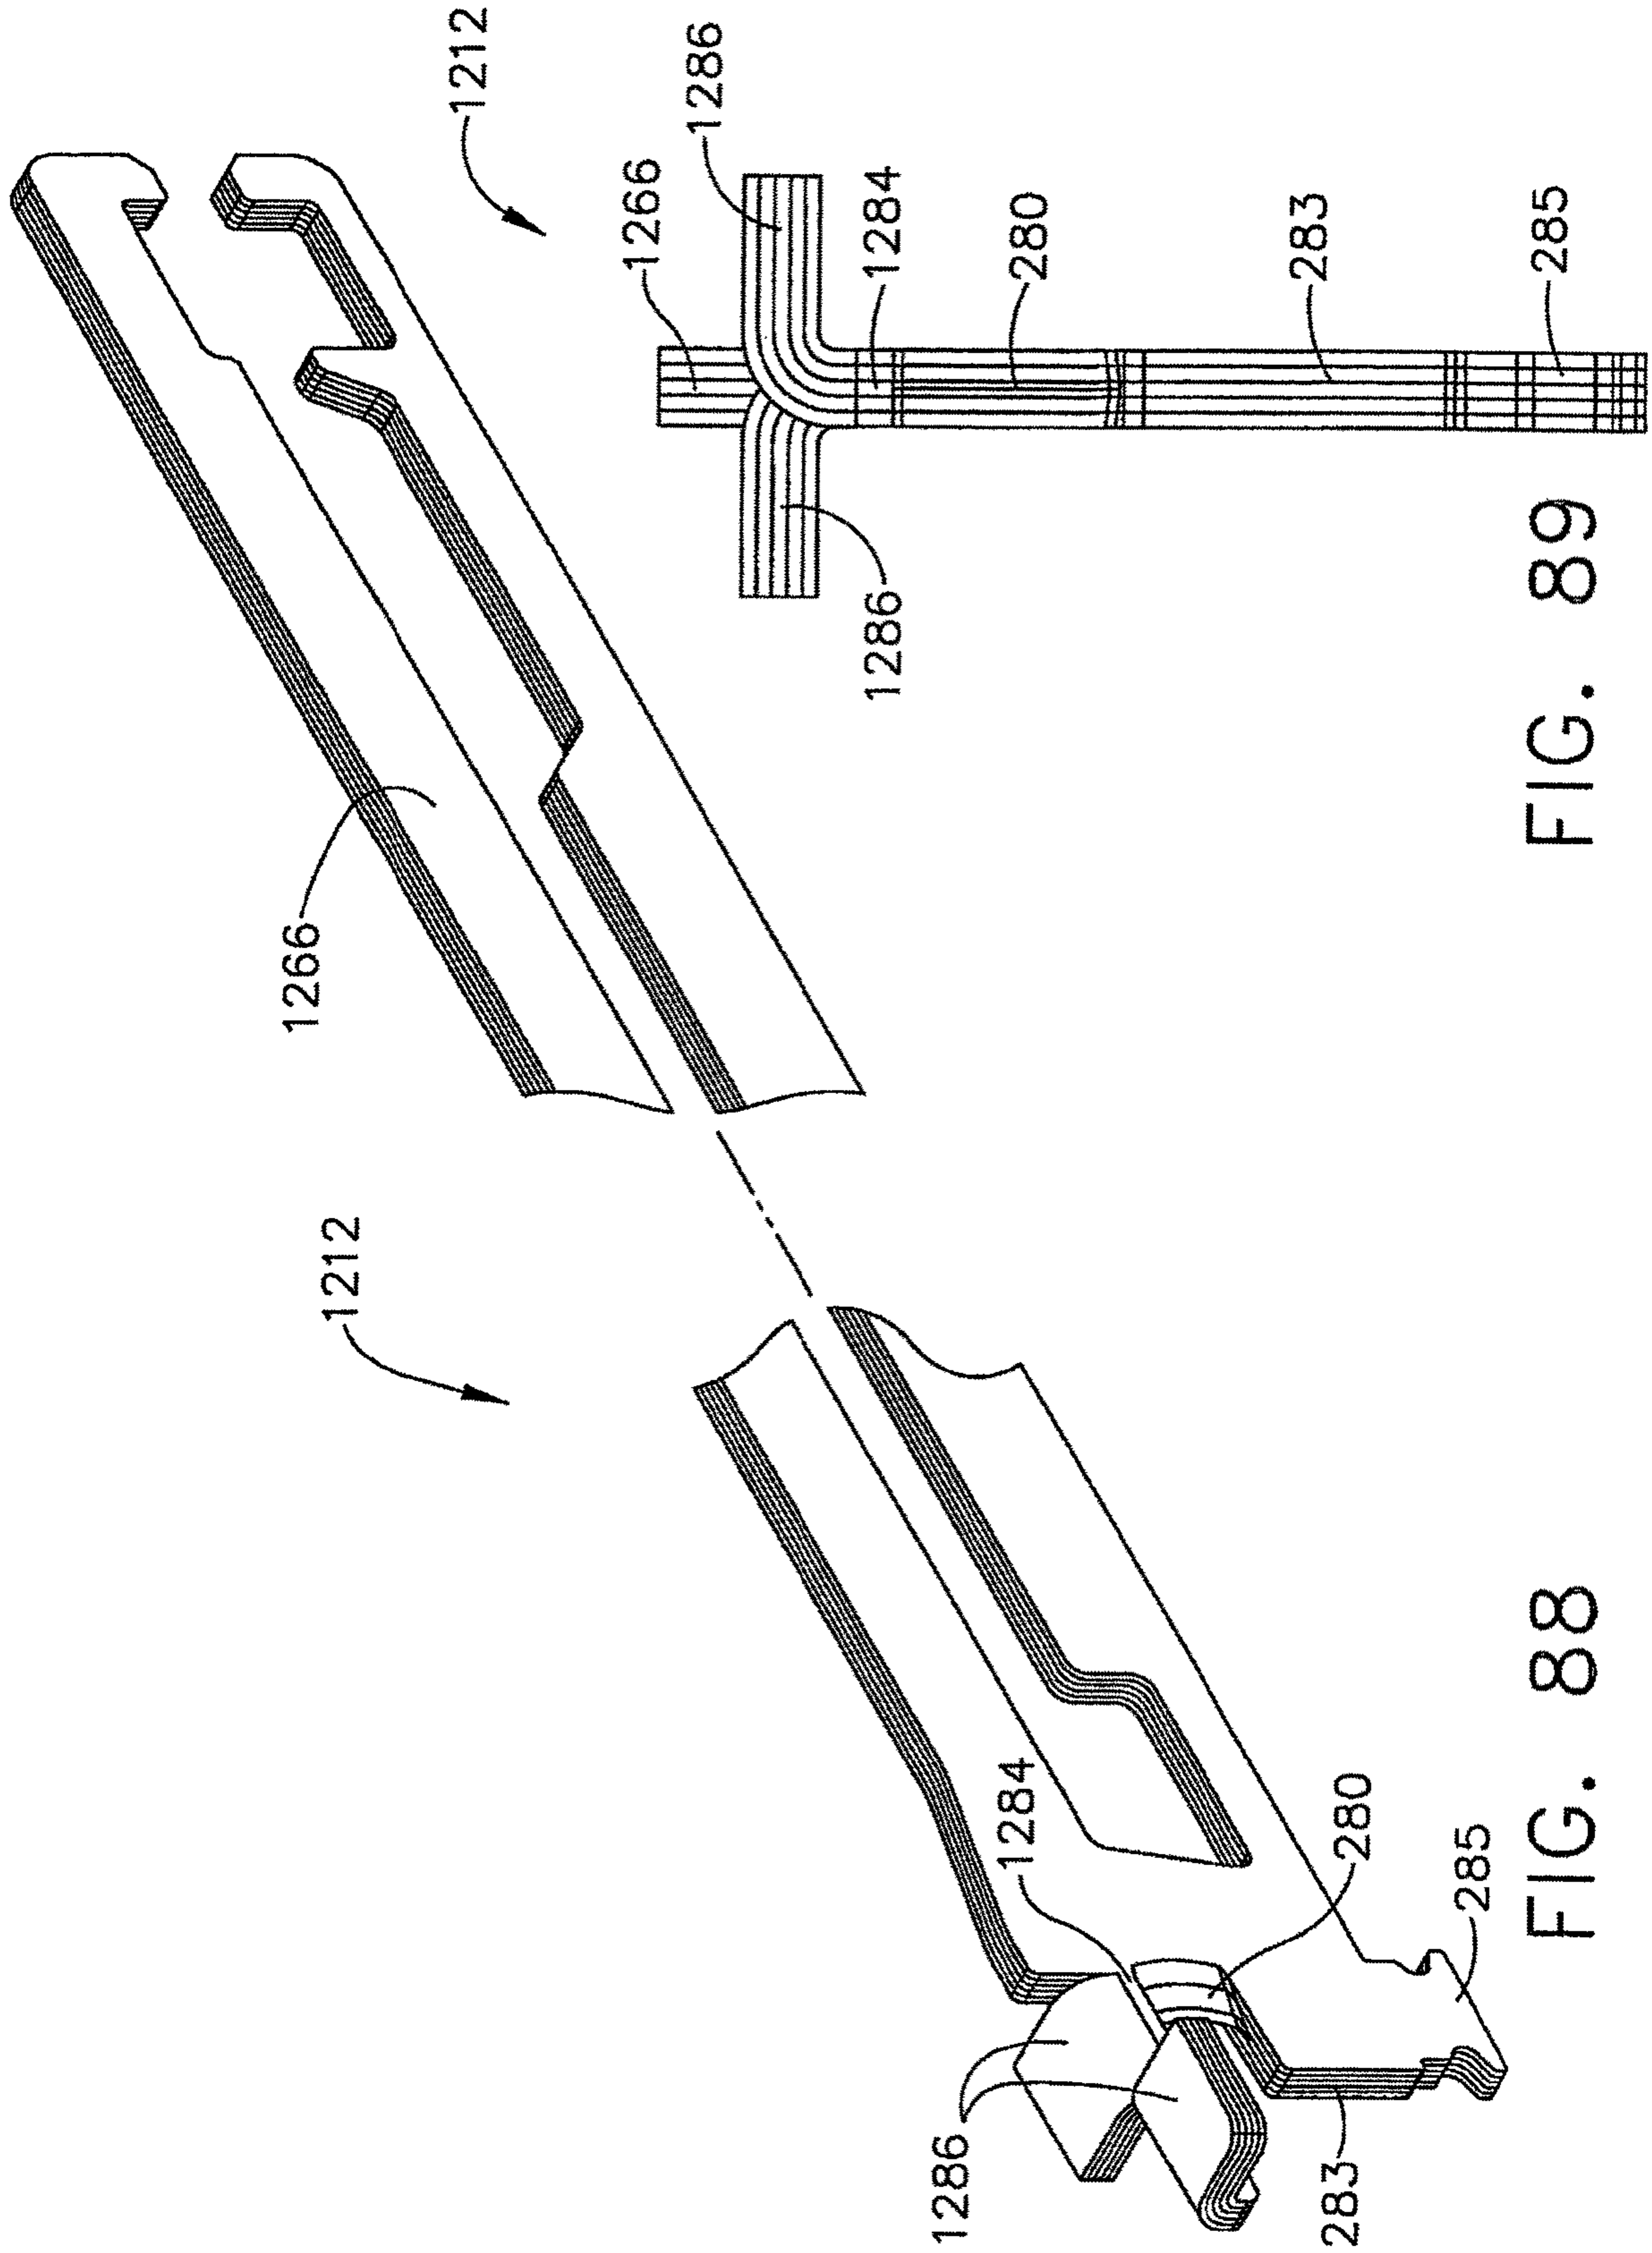


FIG. 89

FIG. 88



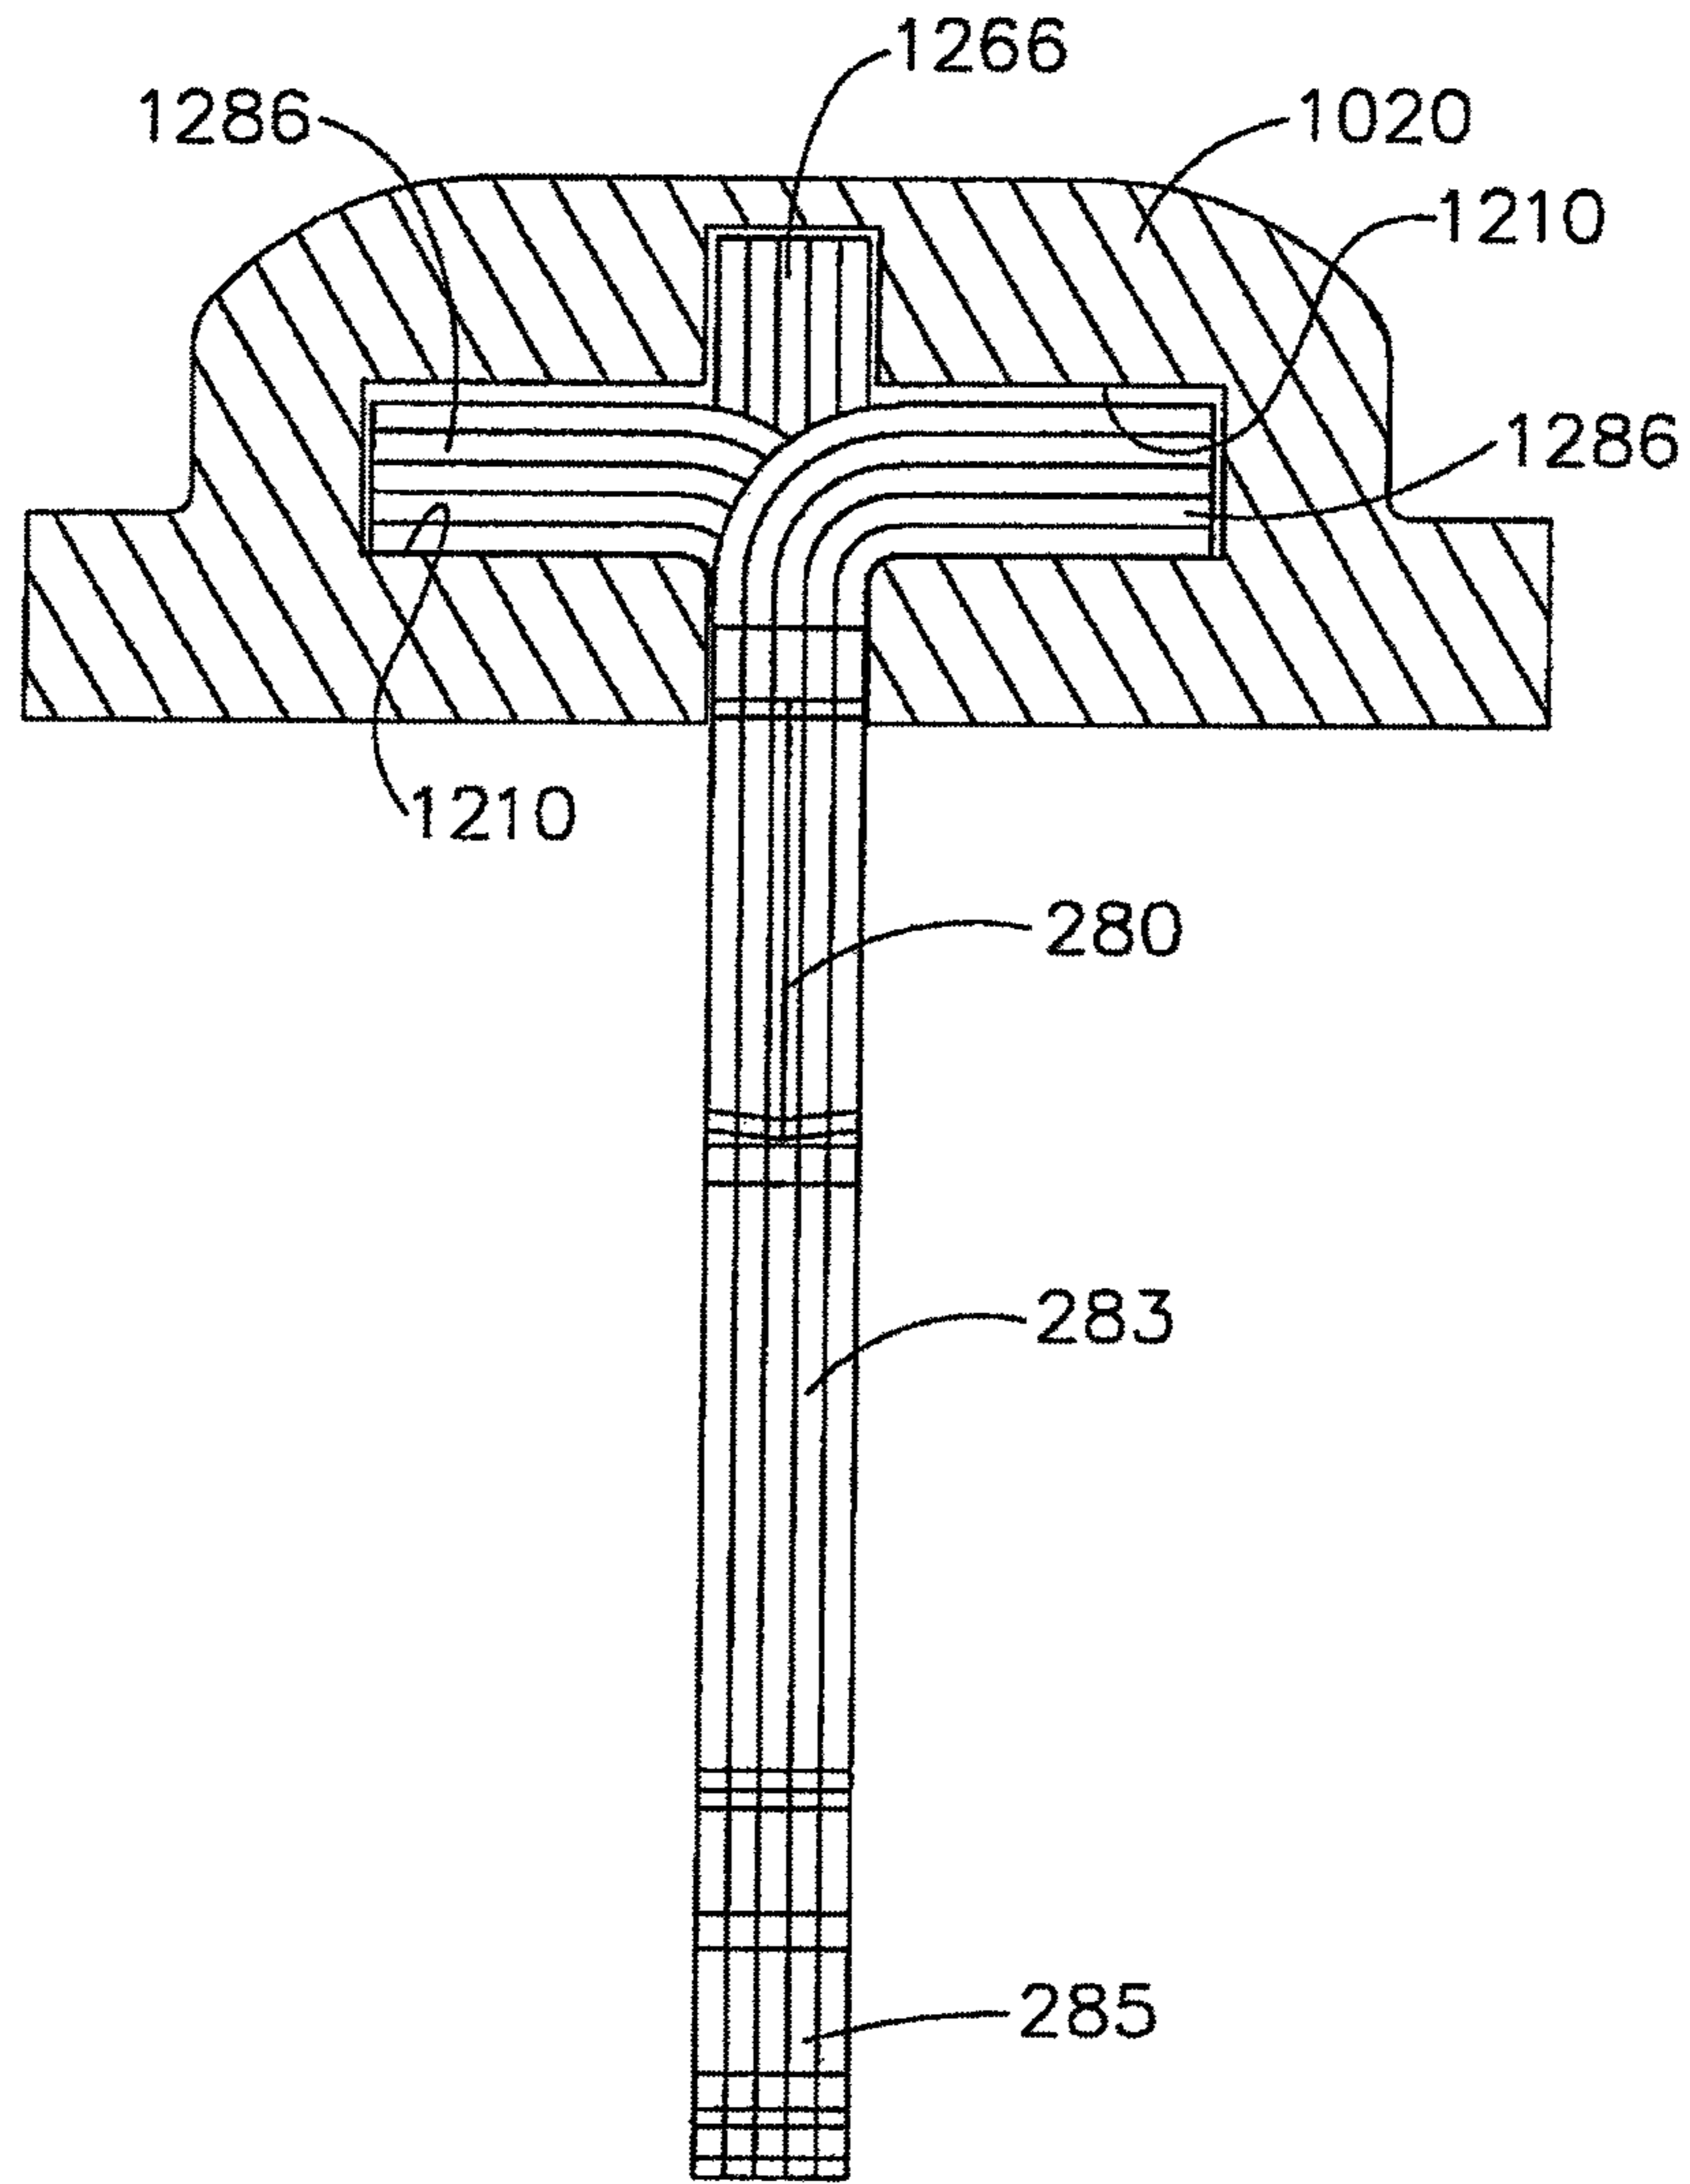


FIG. 90

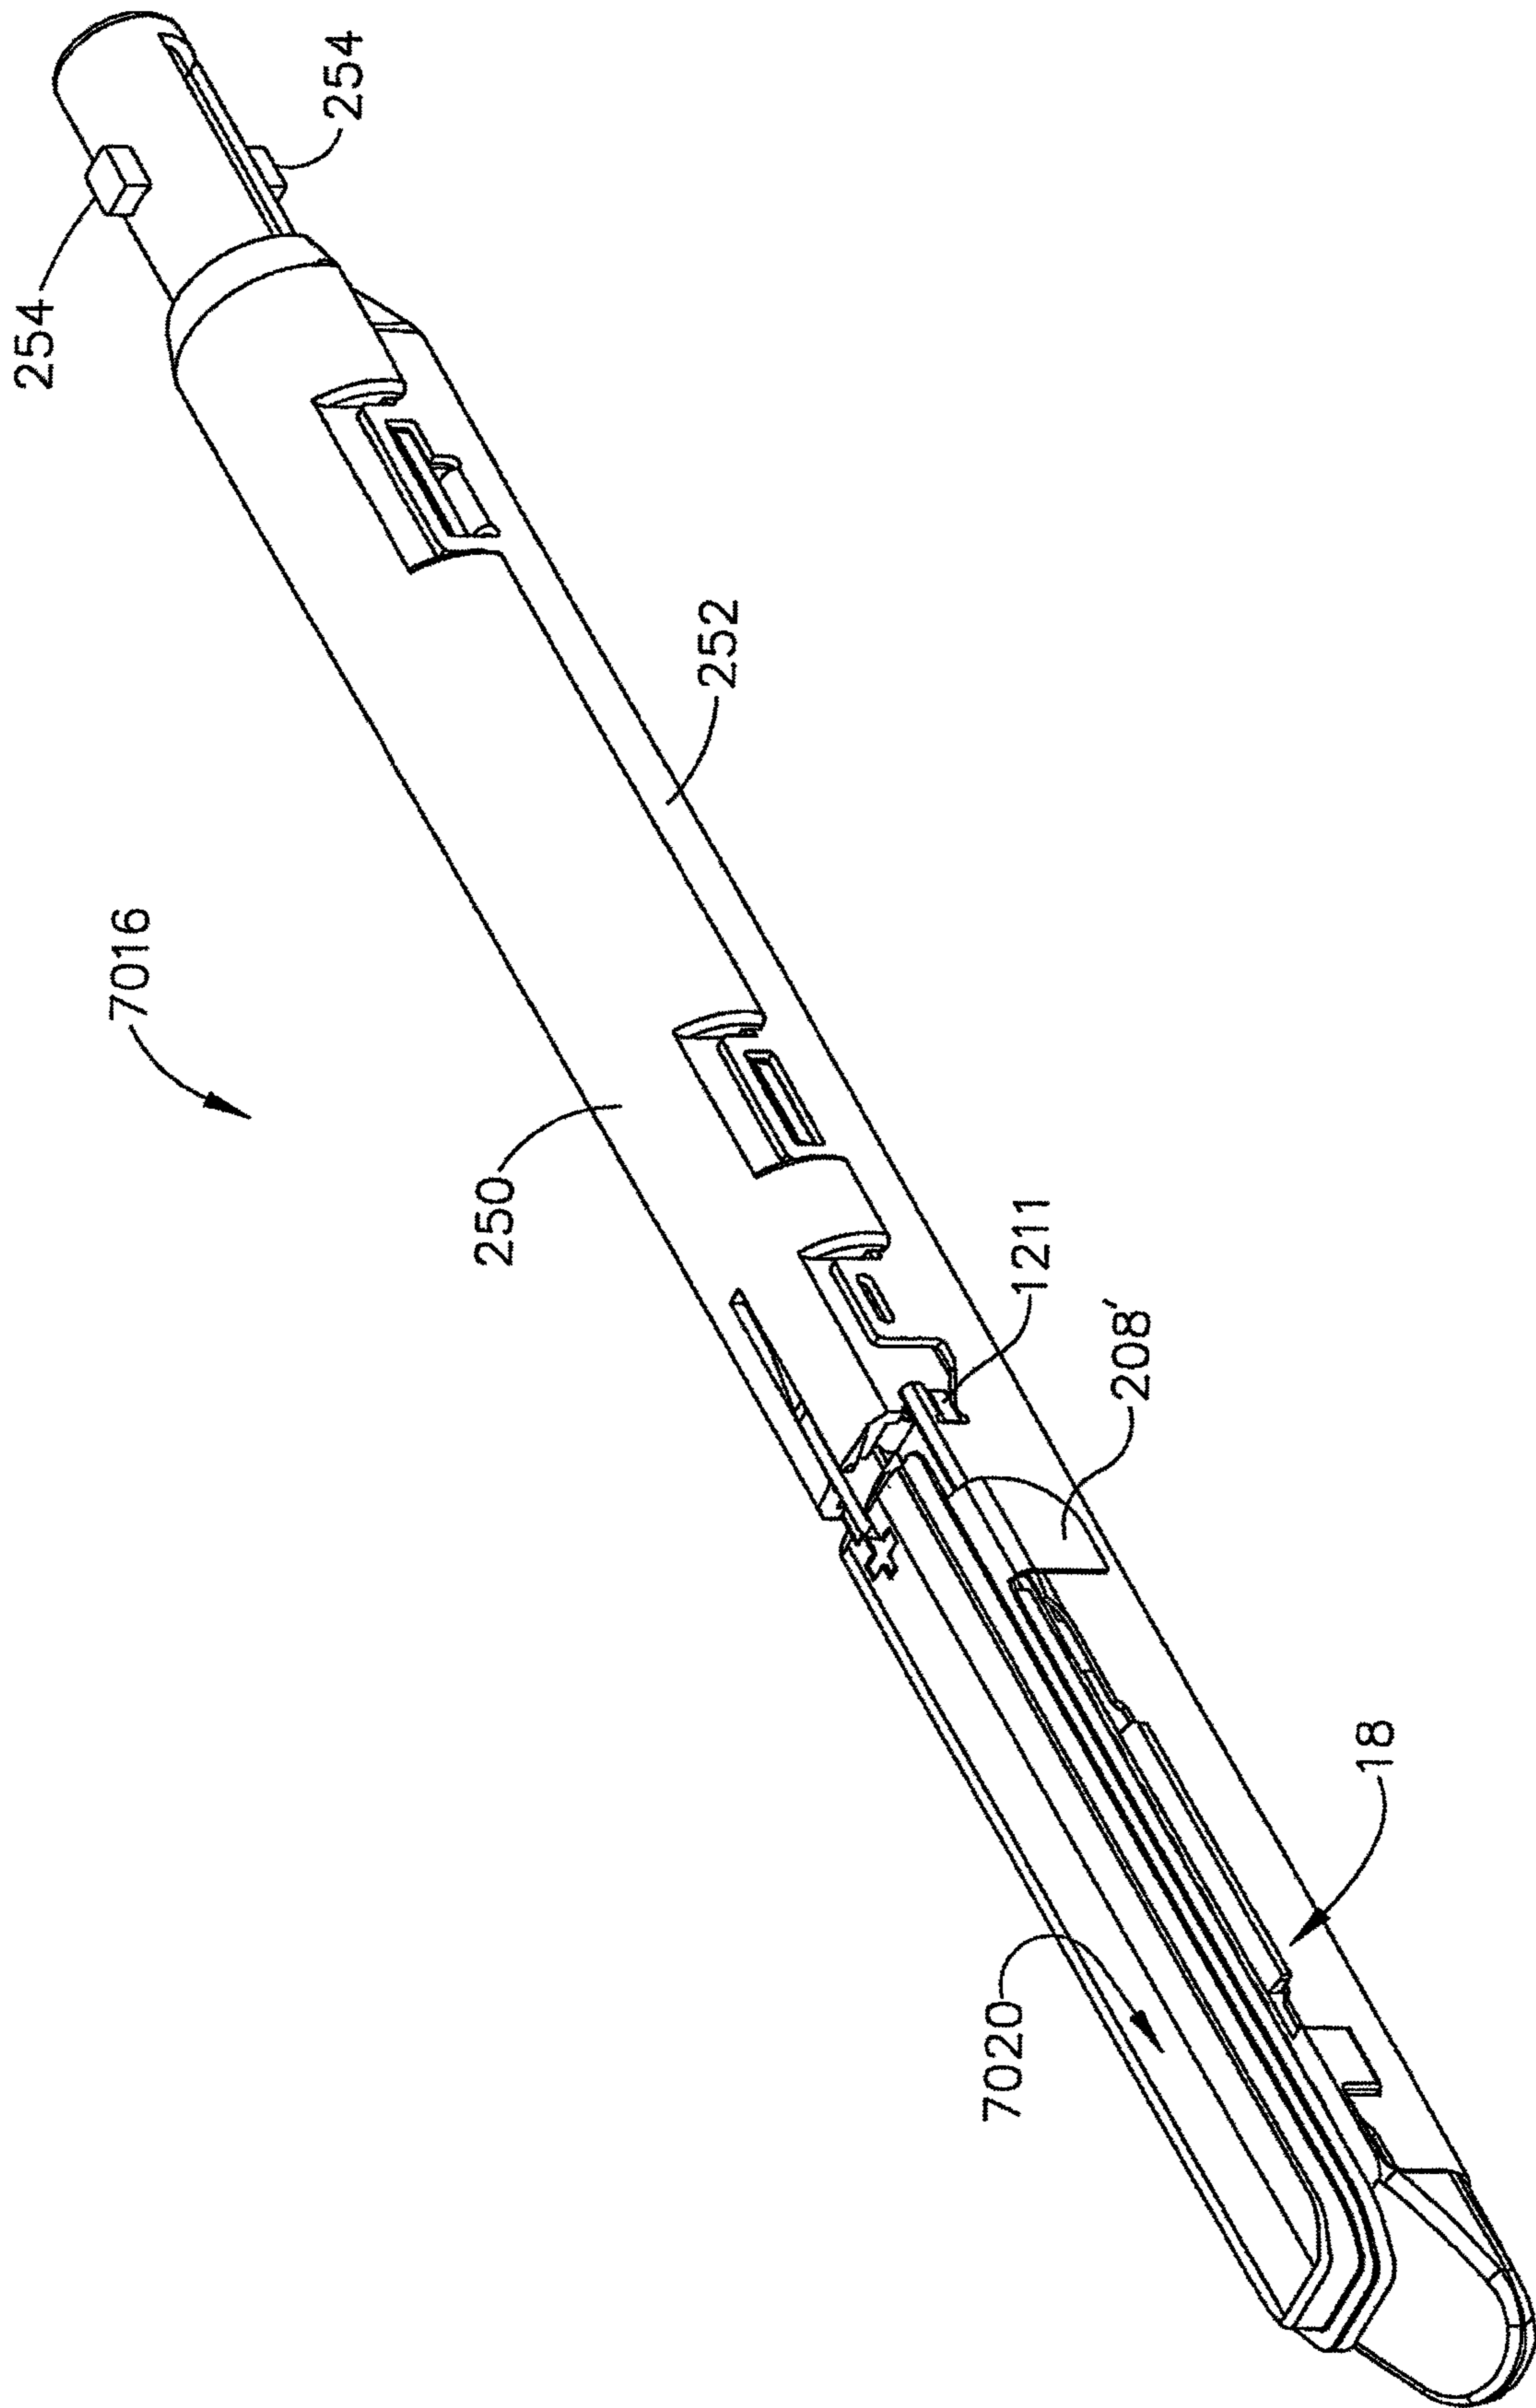


FIG. 91

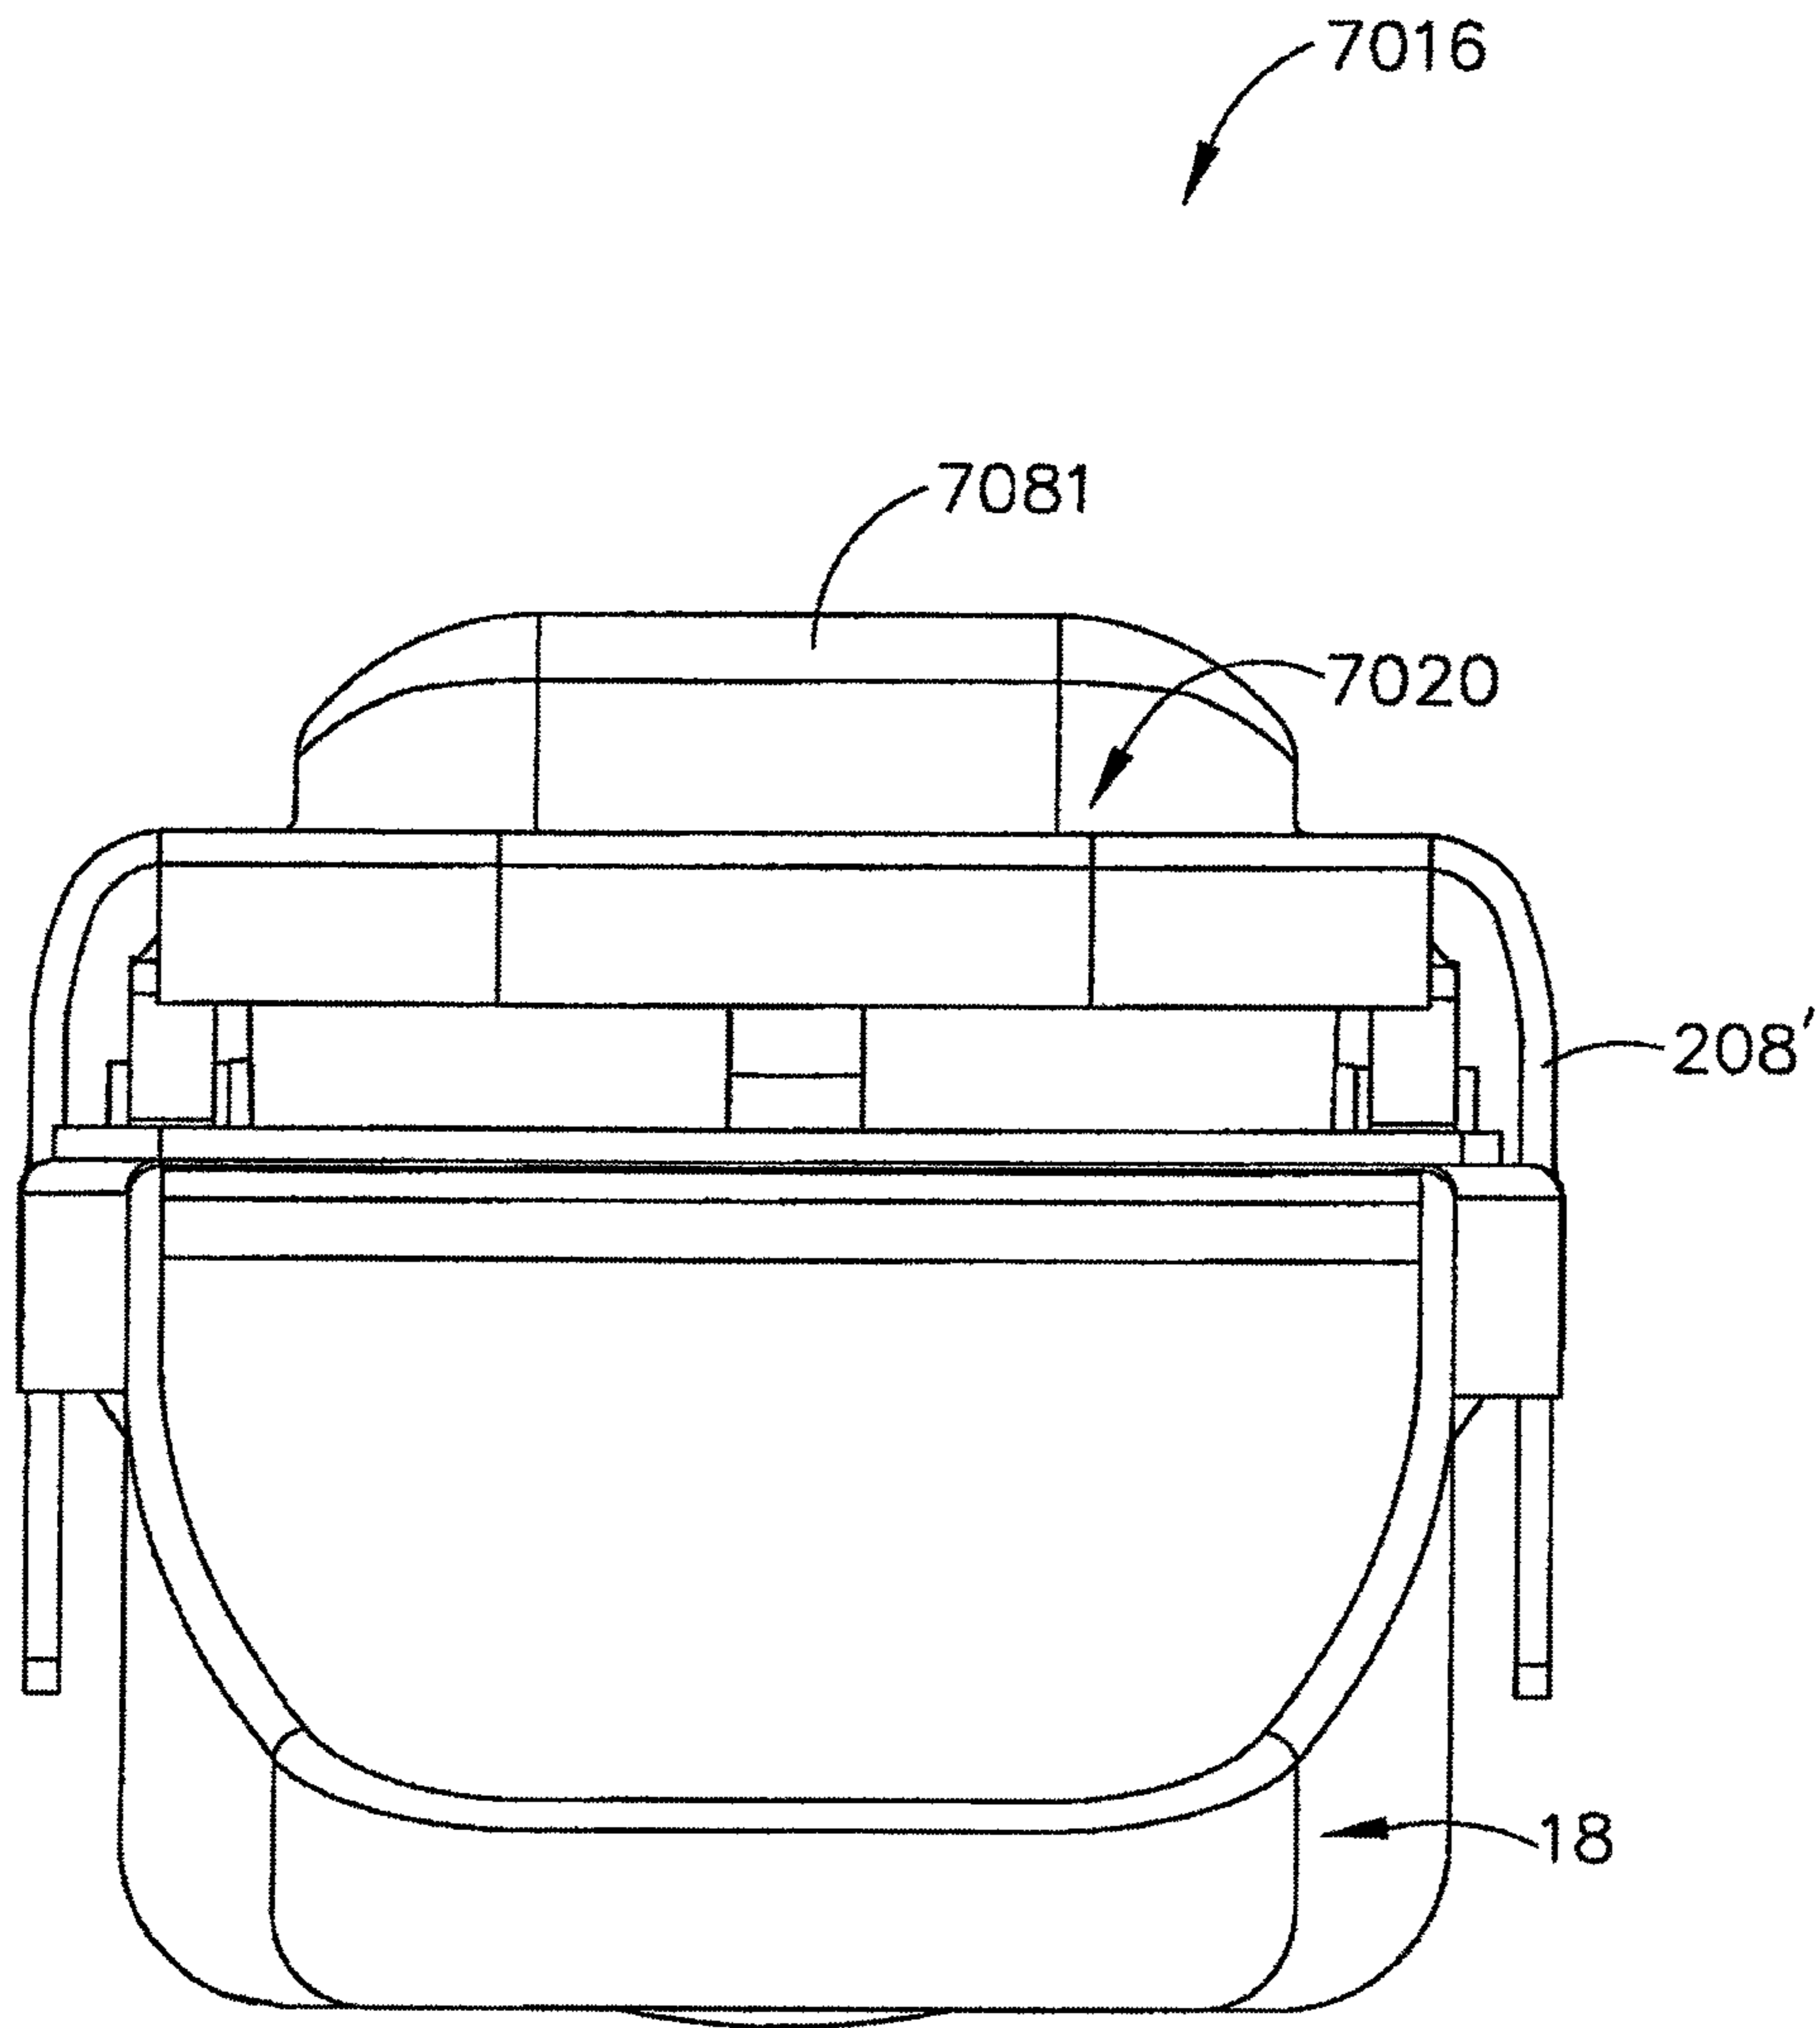


FIG. 92

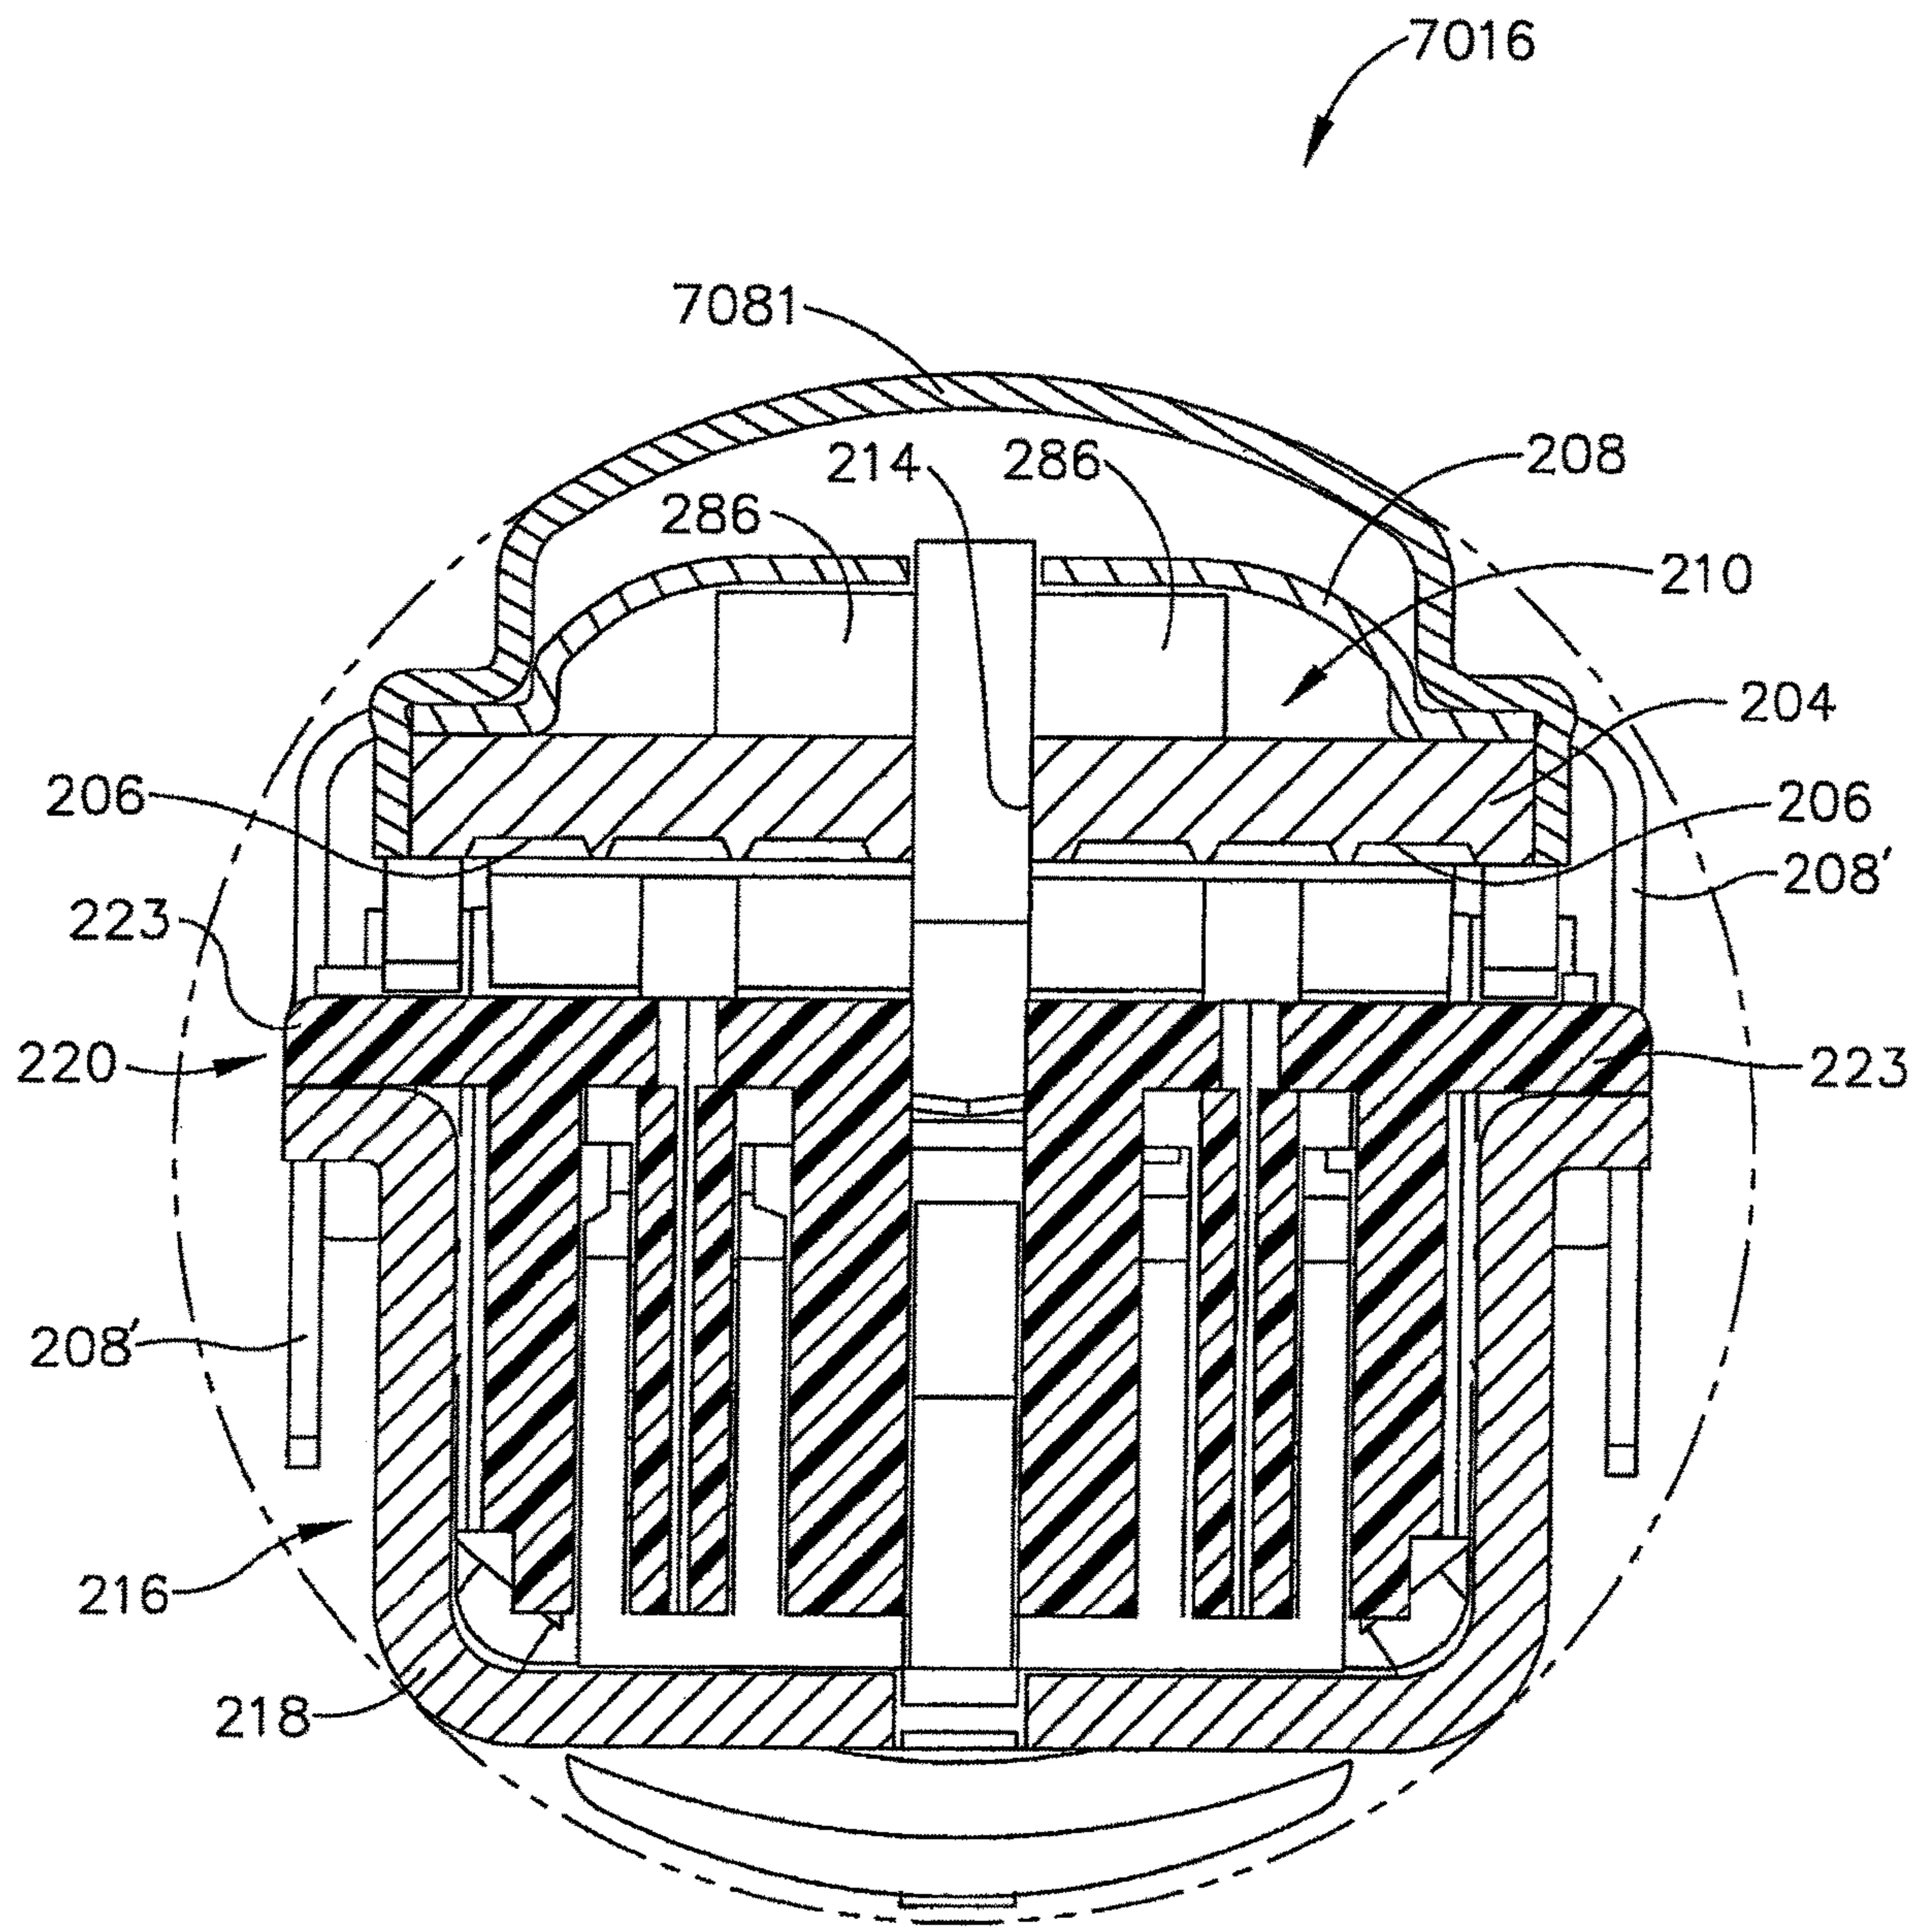


FIG. 93

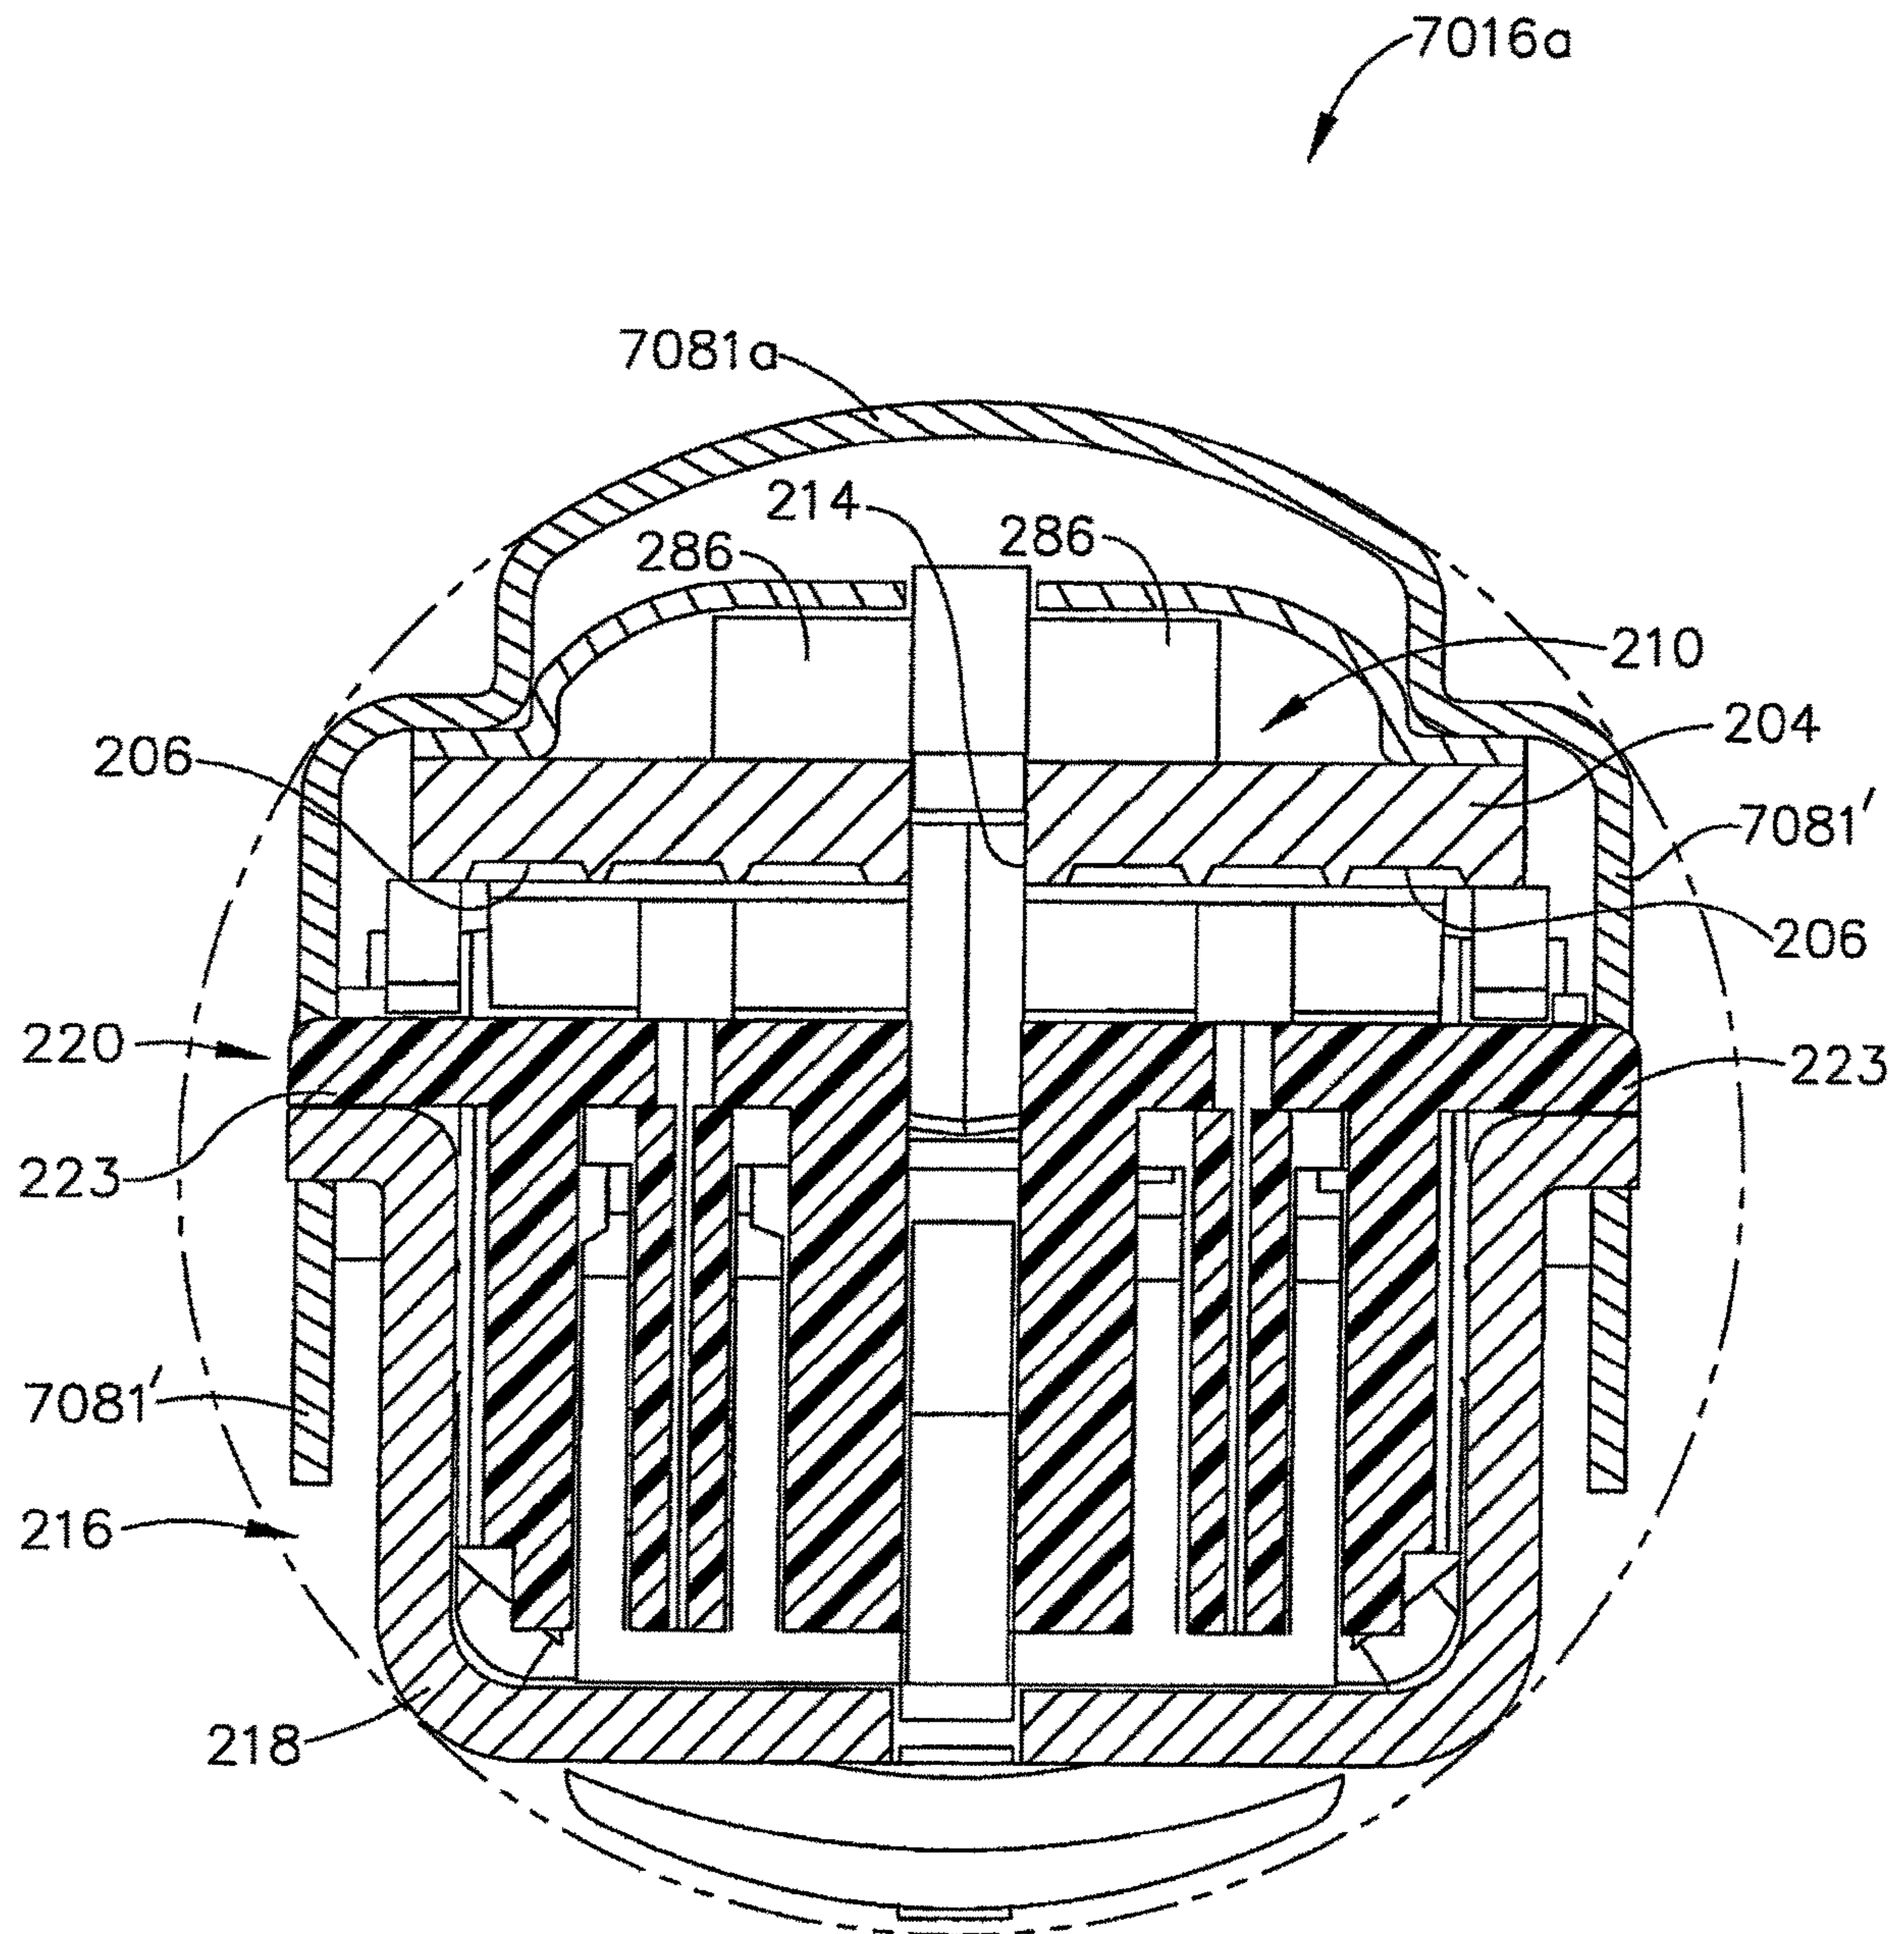


FIG. 94

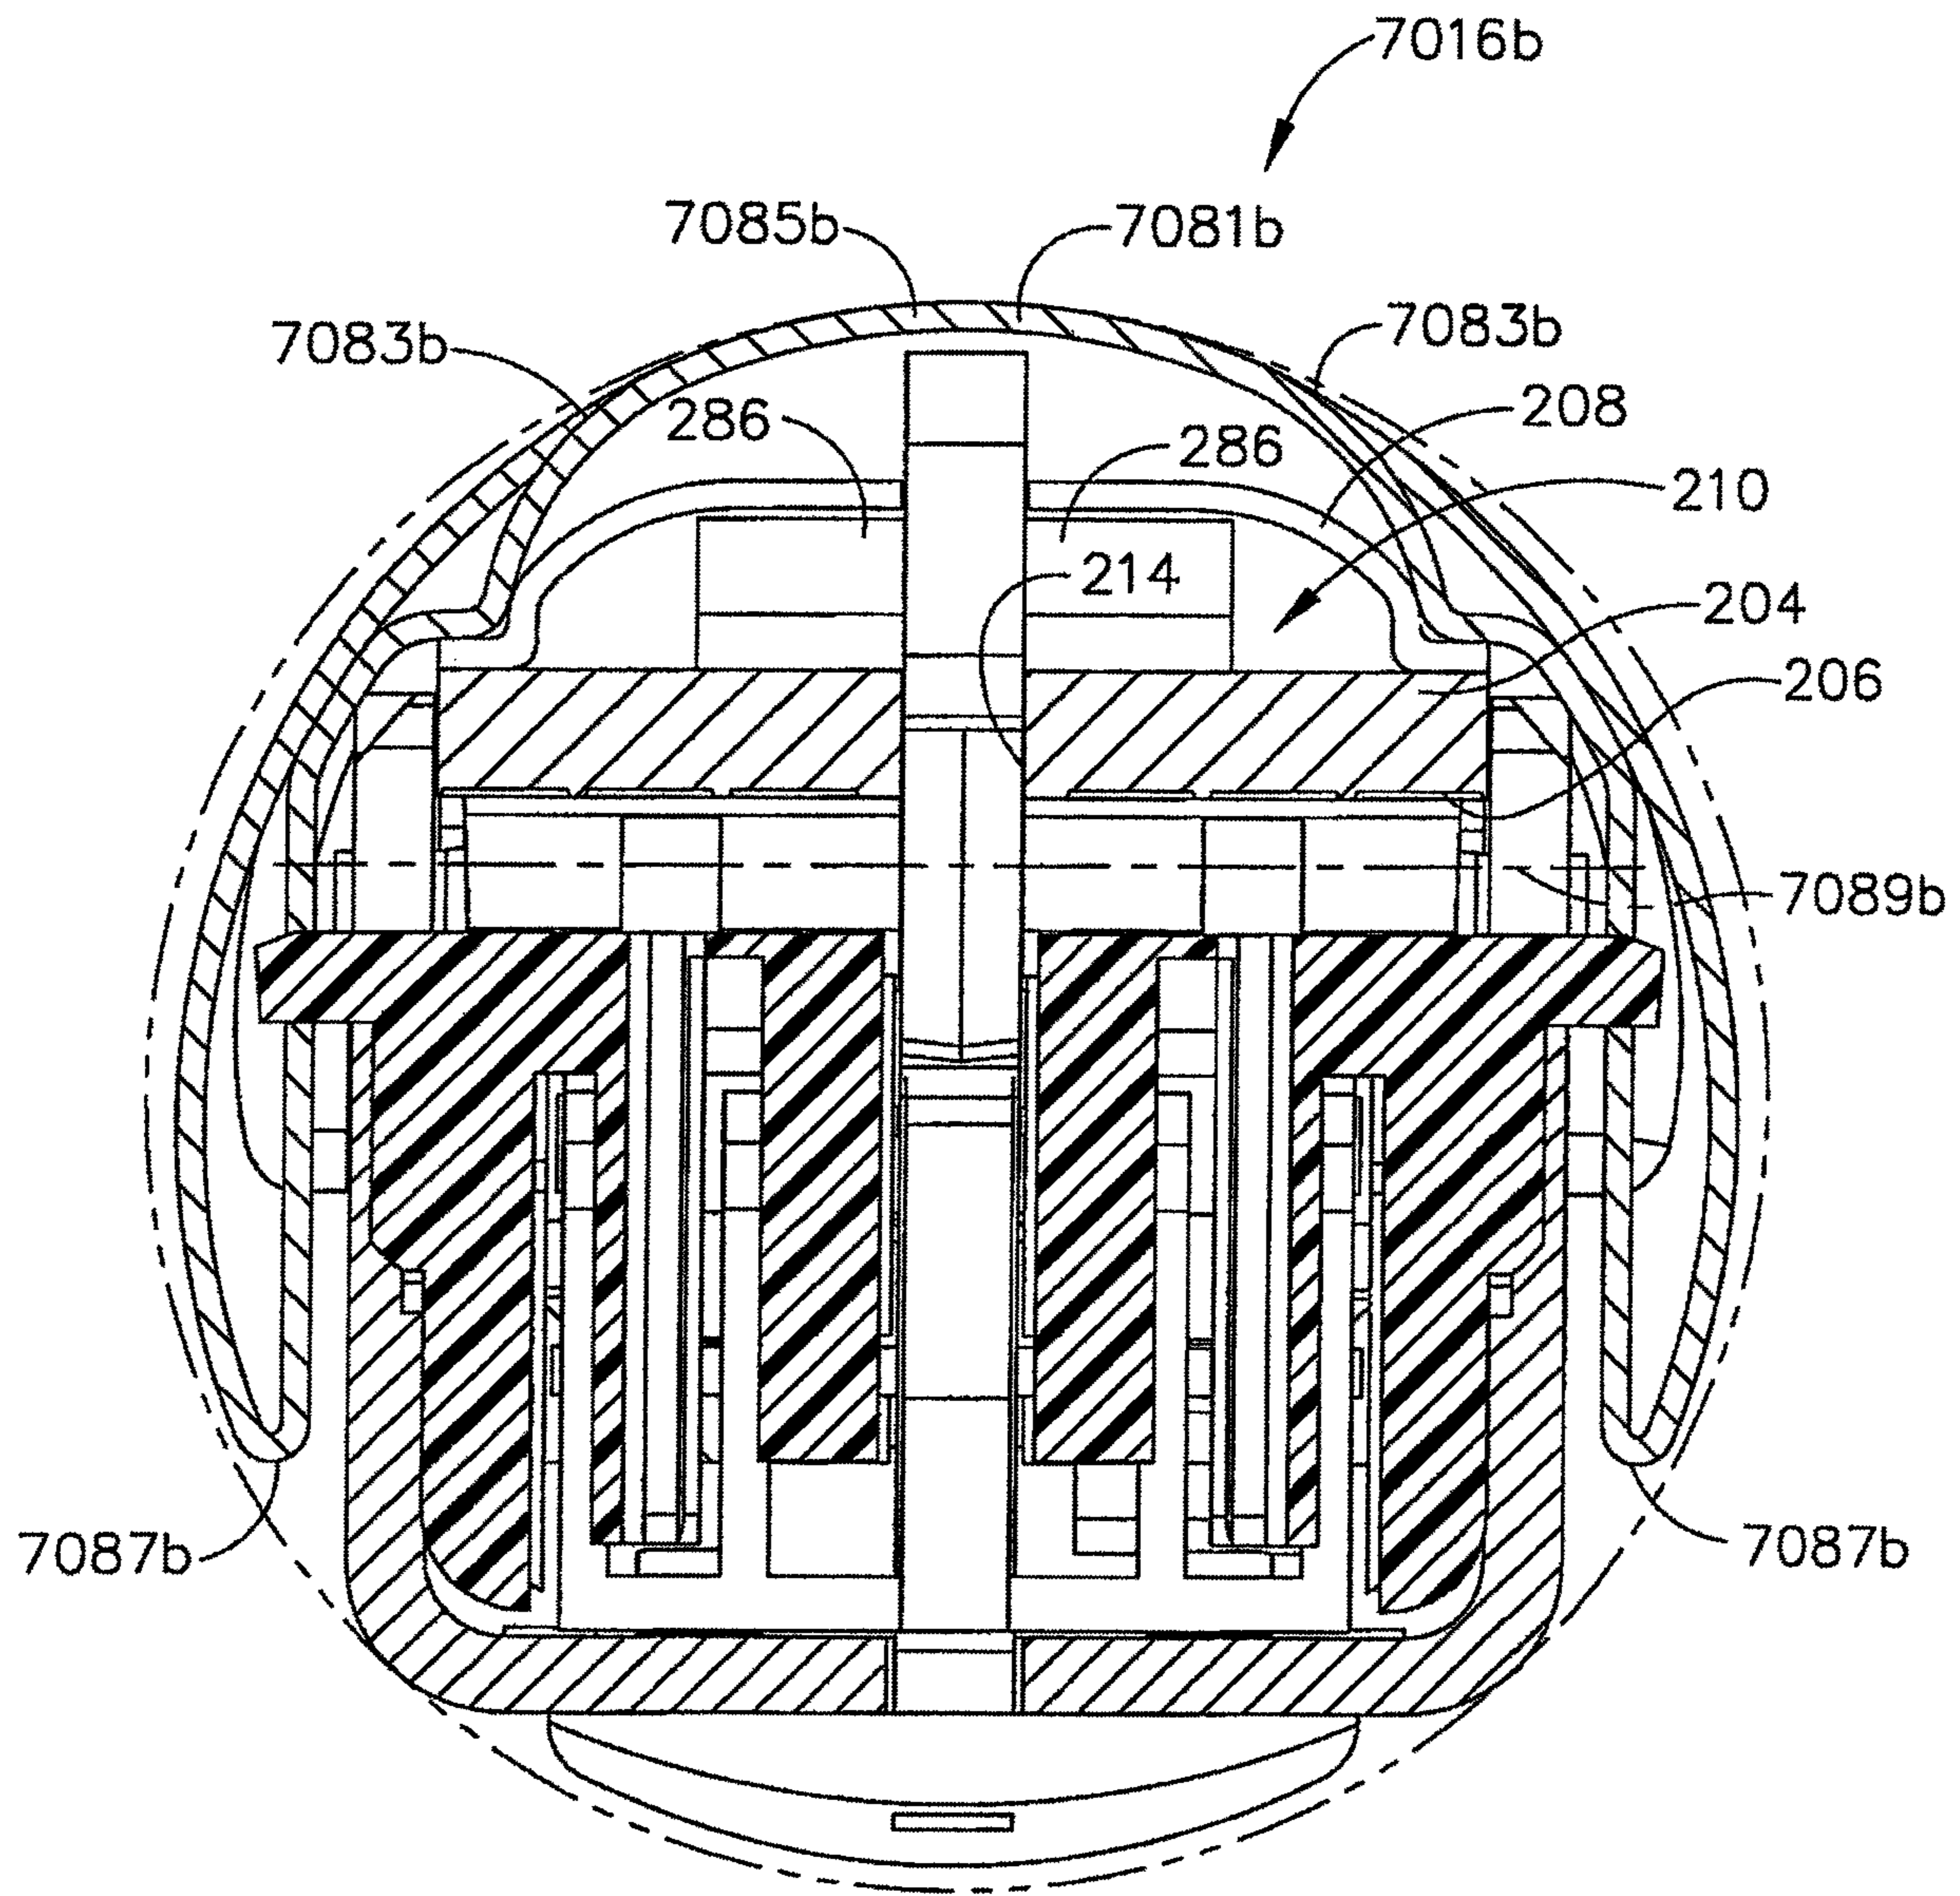


FIG. 95

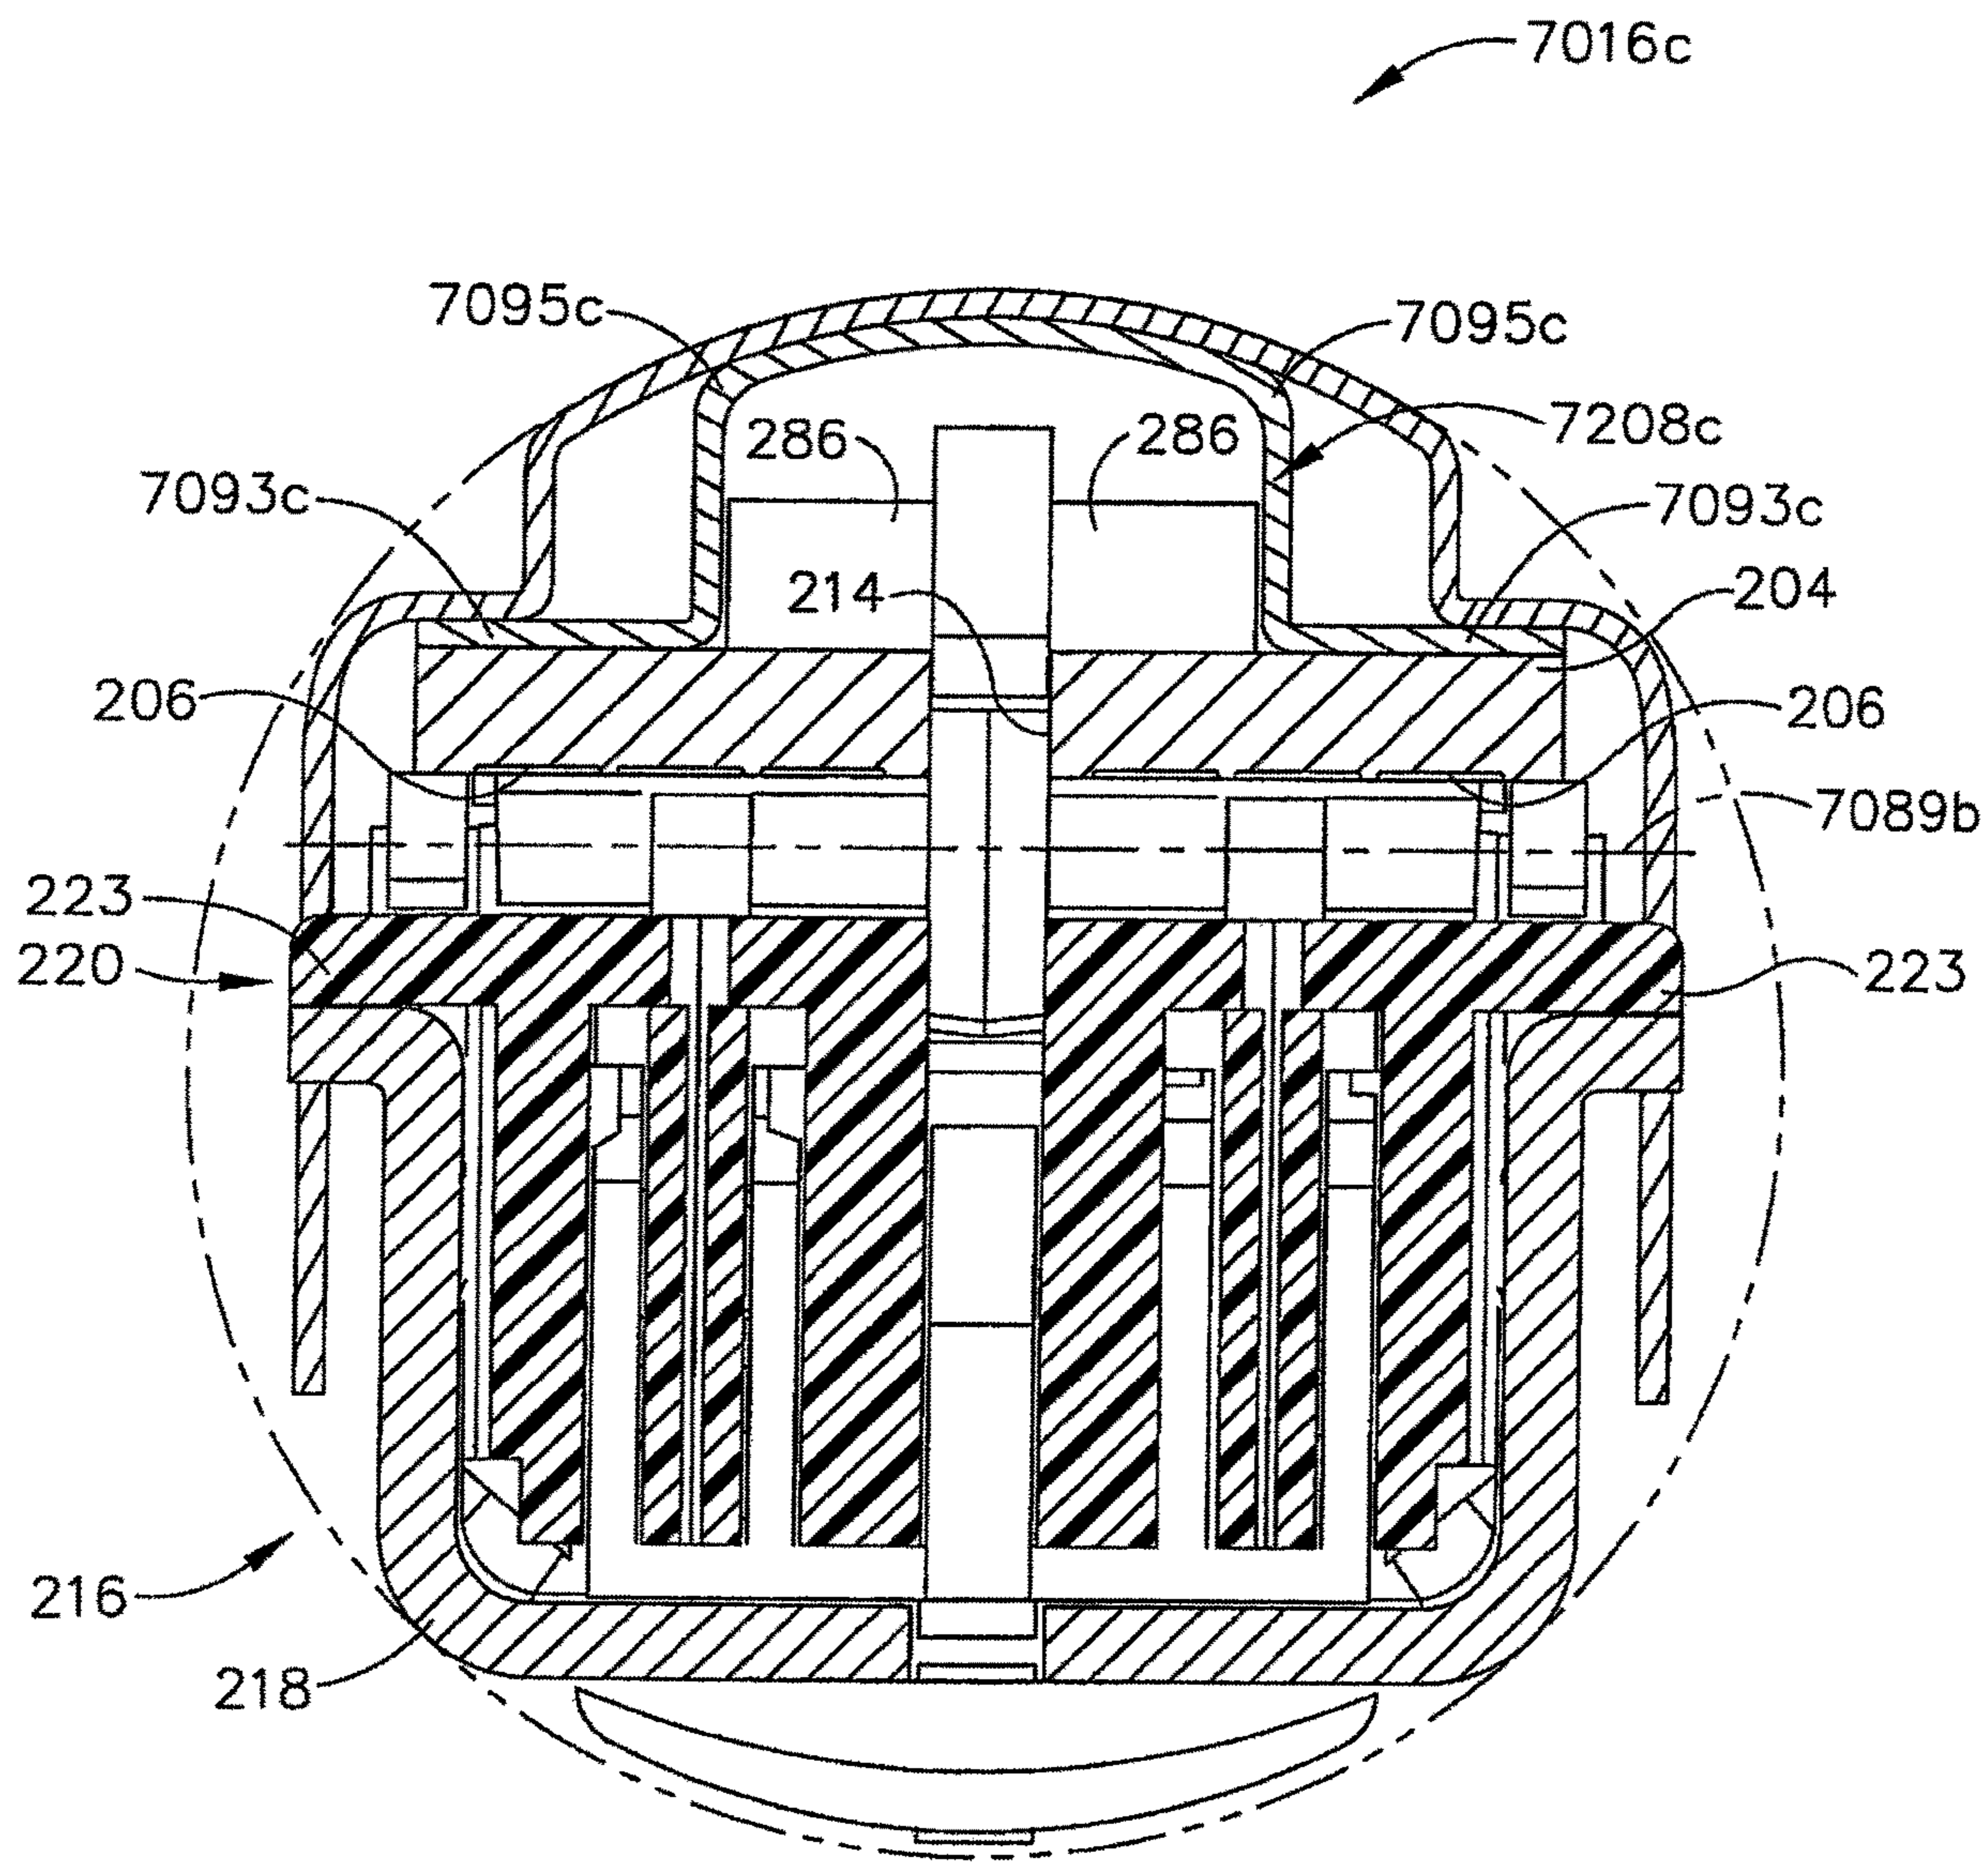


FIG. 96

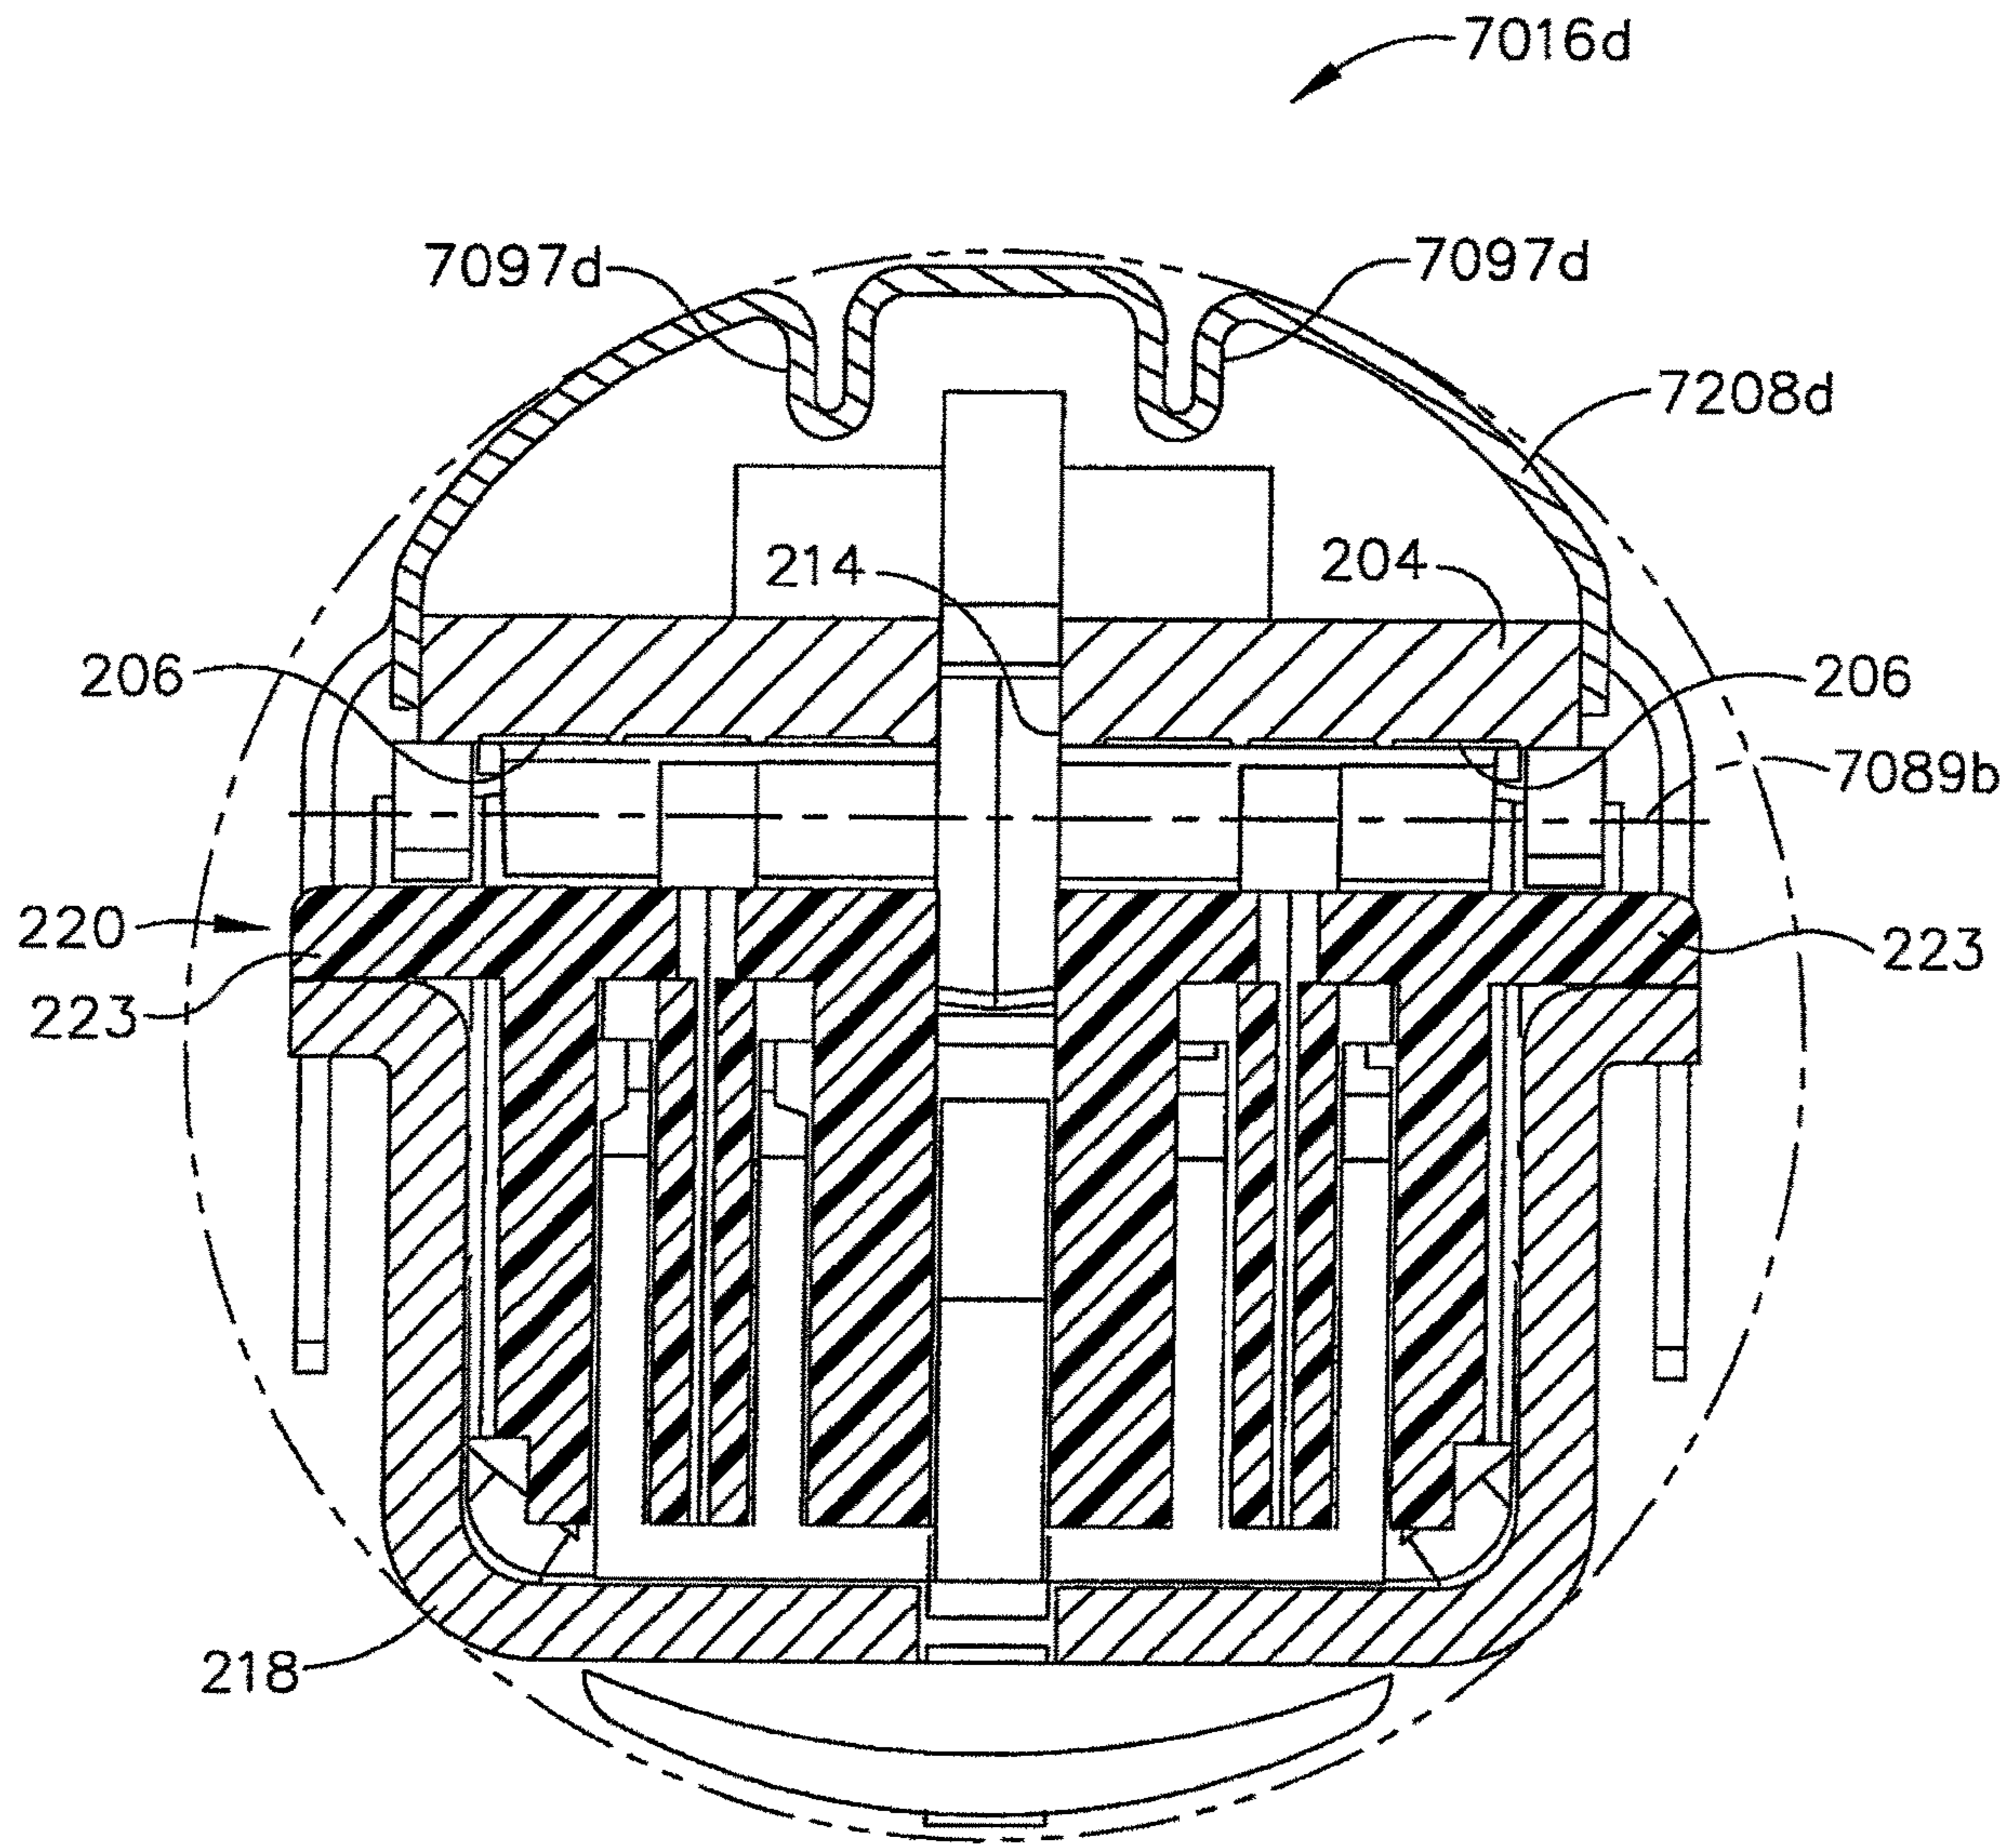


FIG. 97



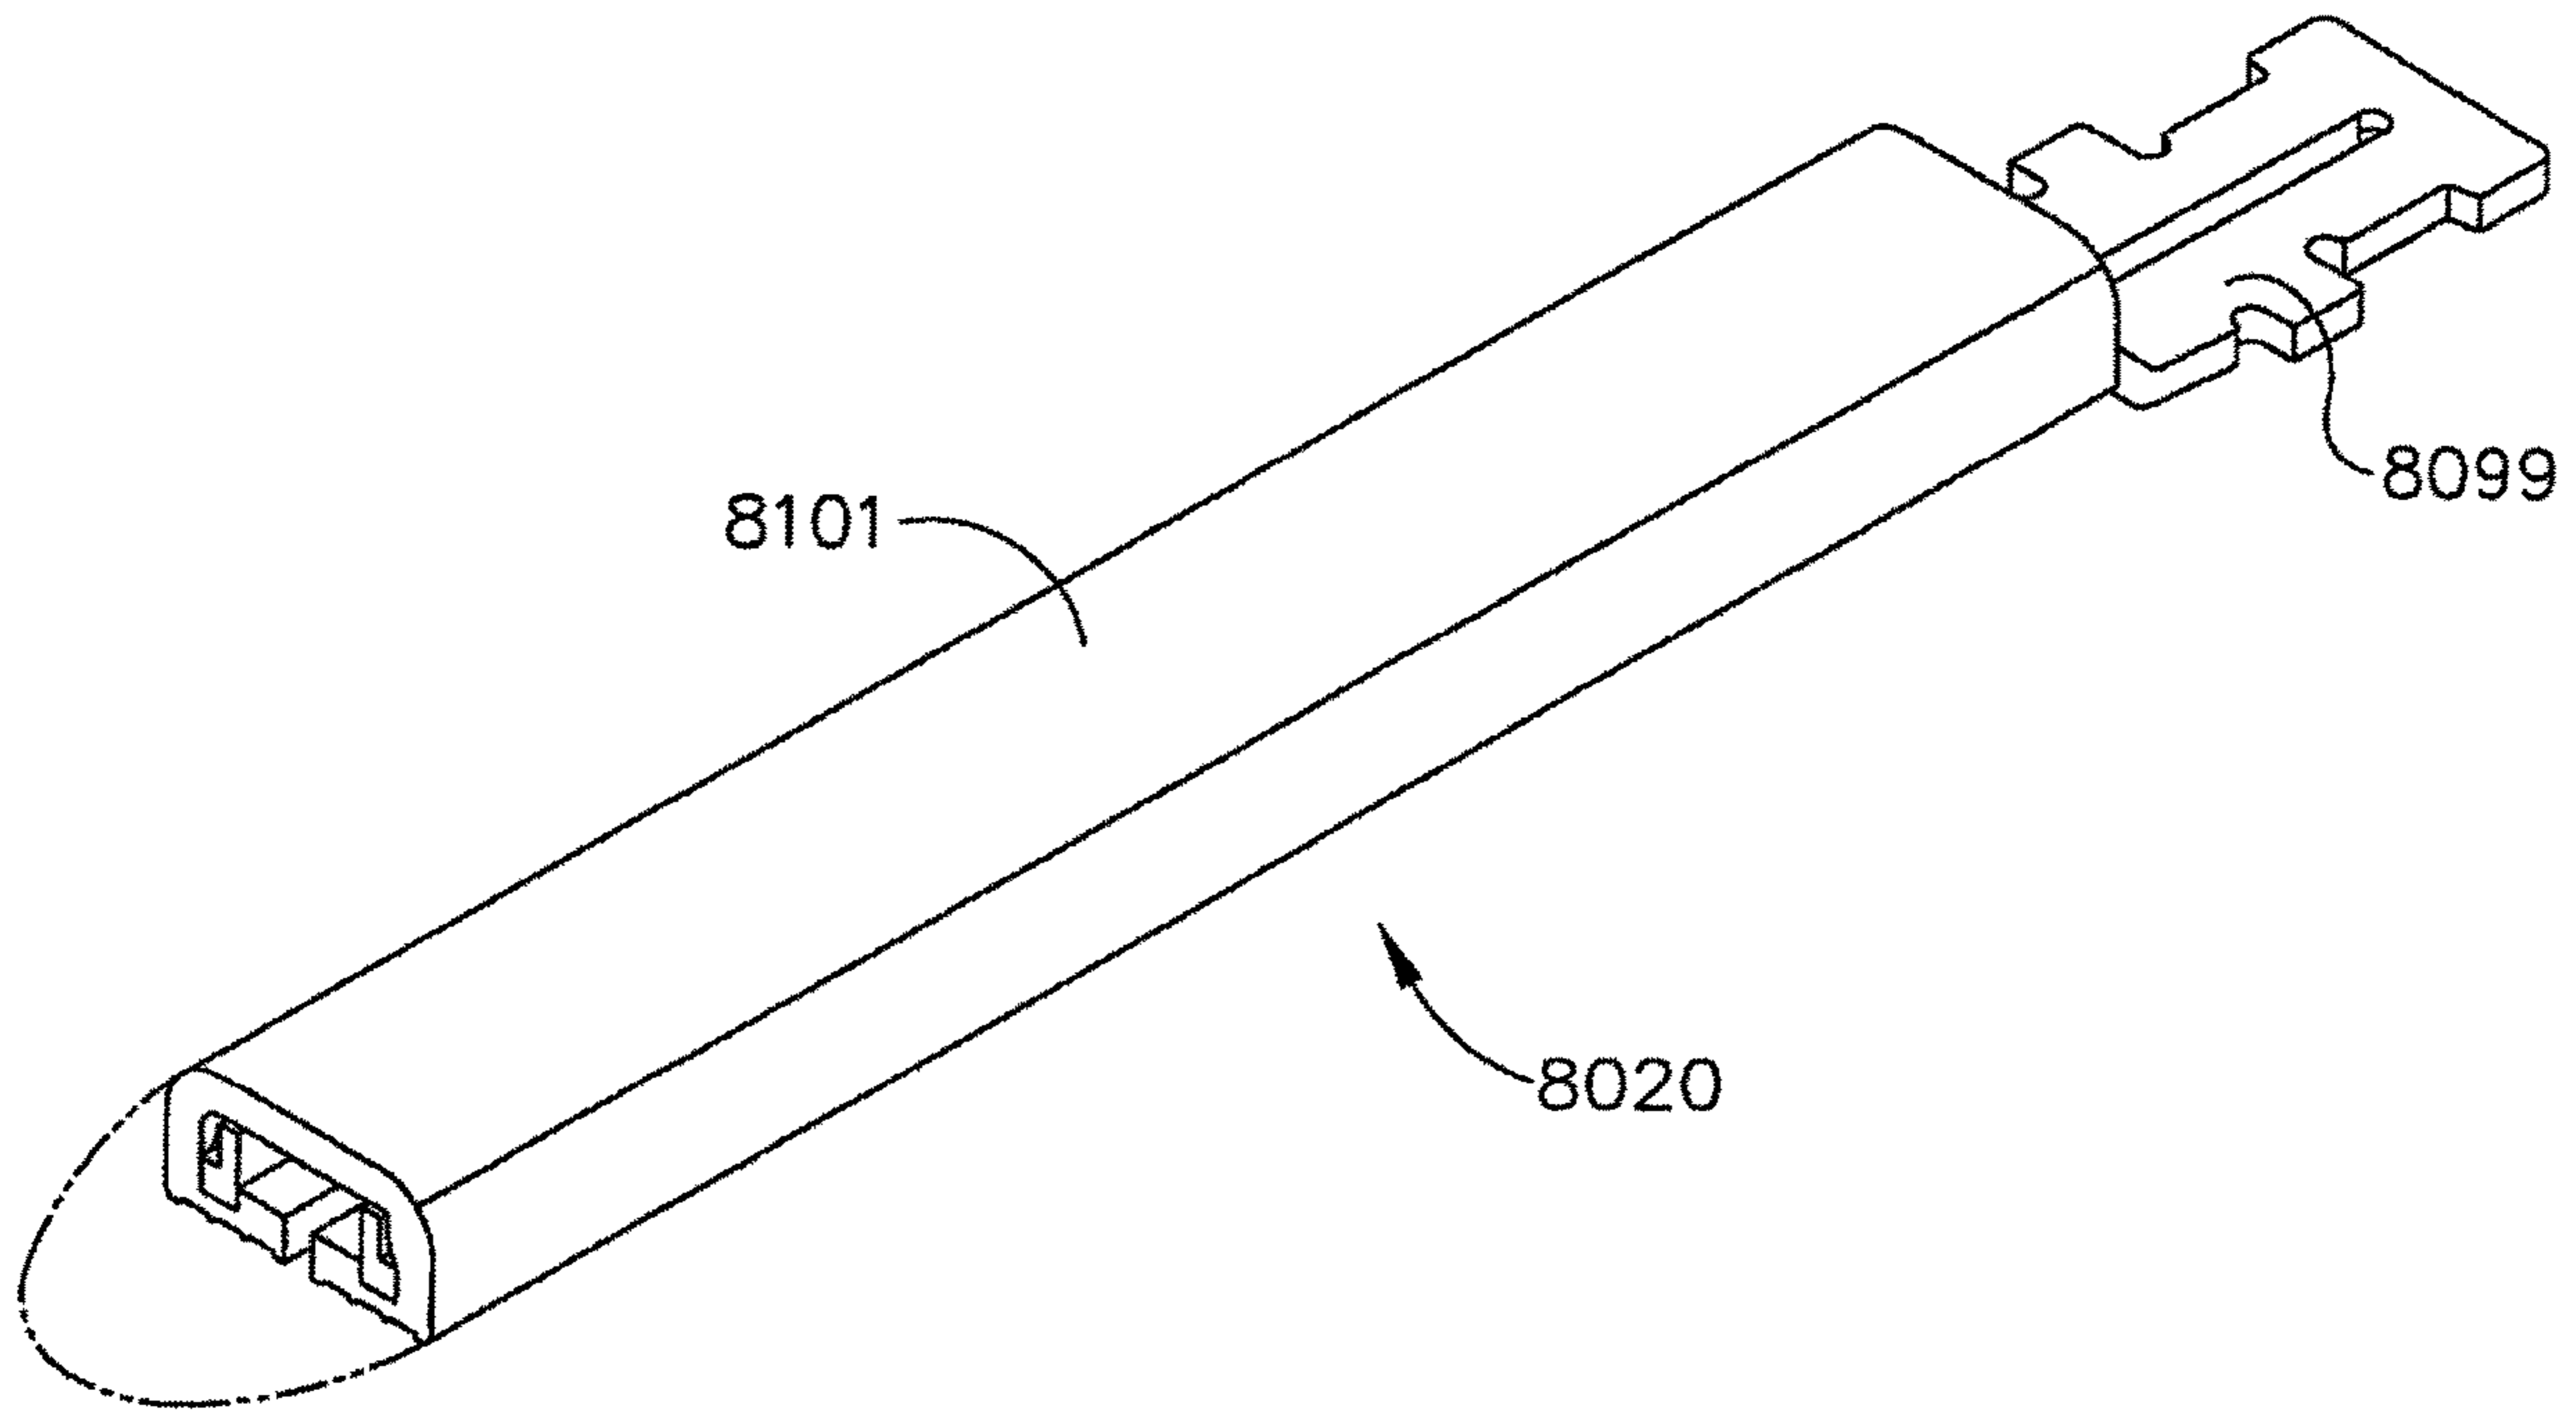


FIG. 98

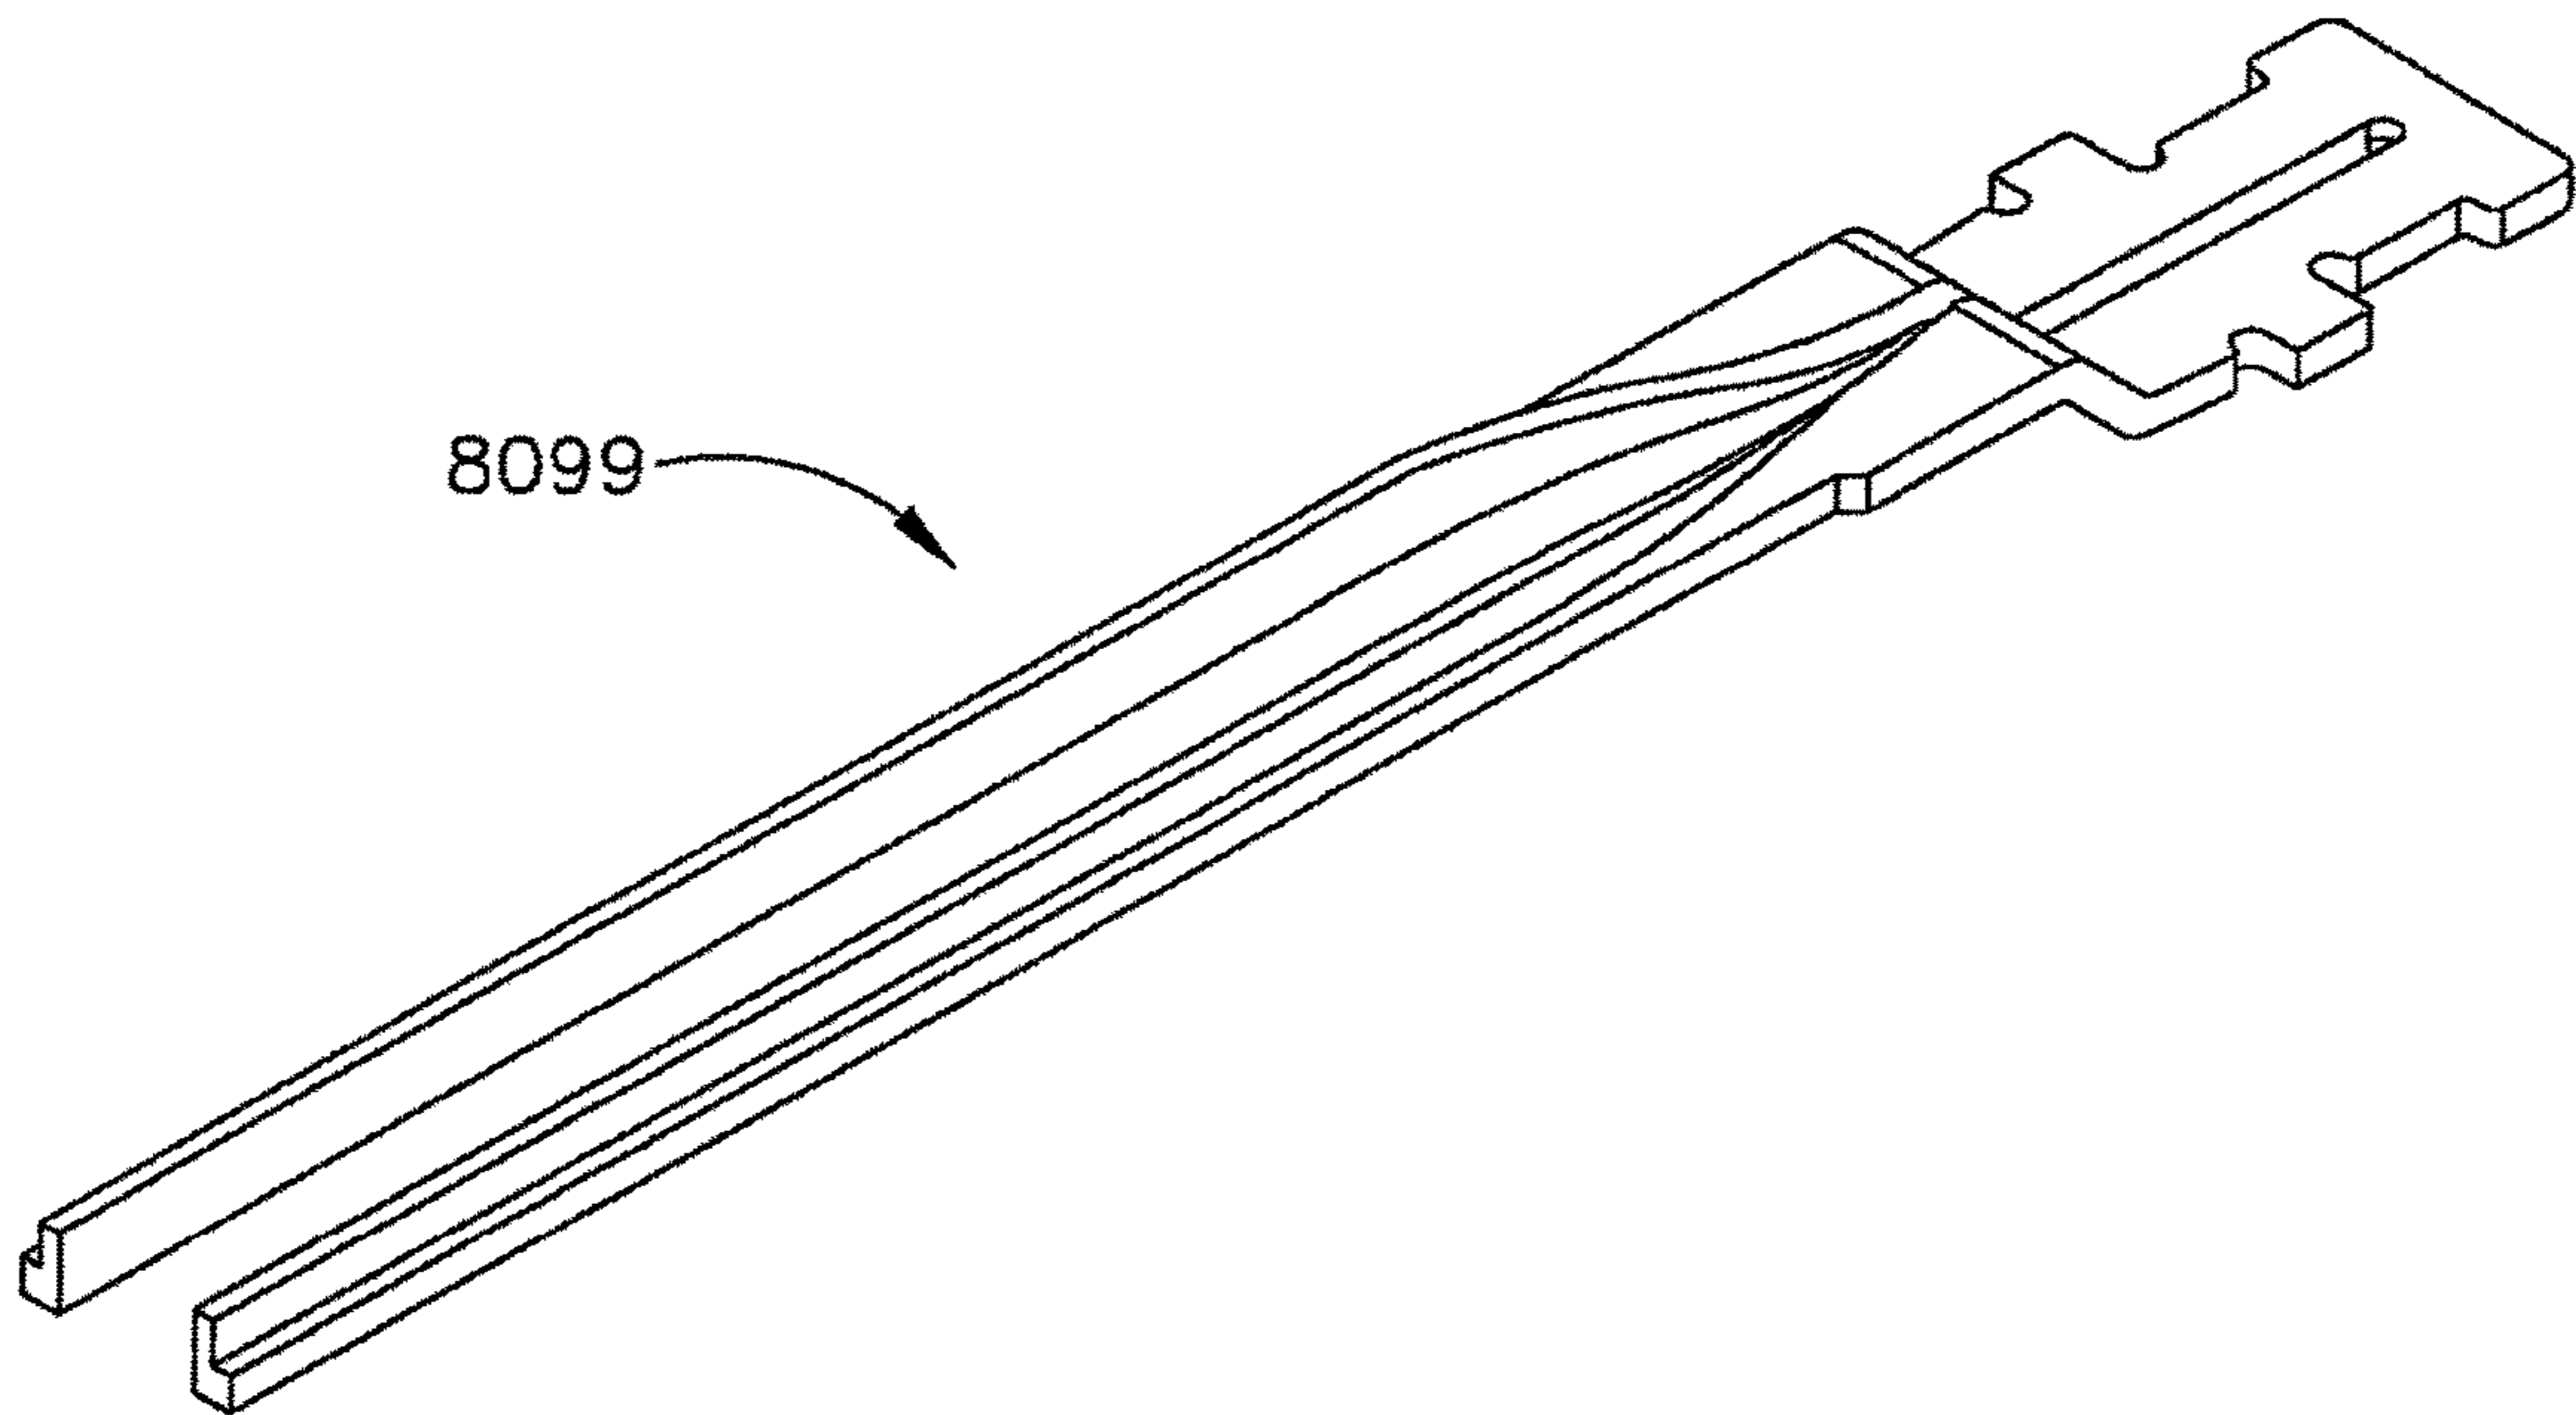


FIG. 99

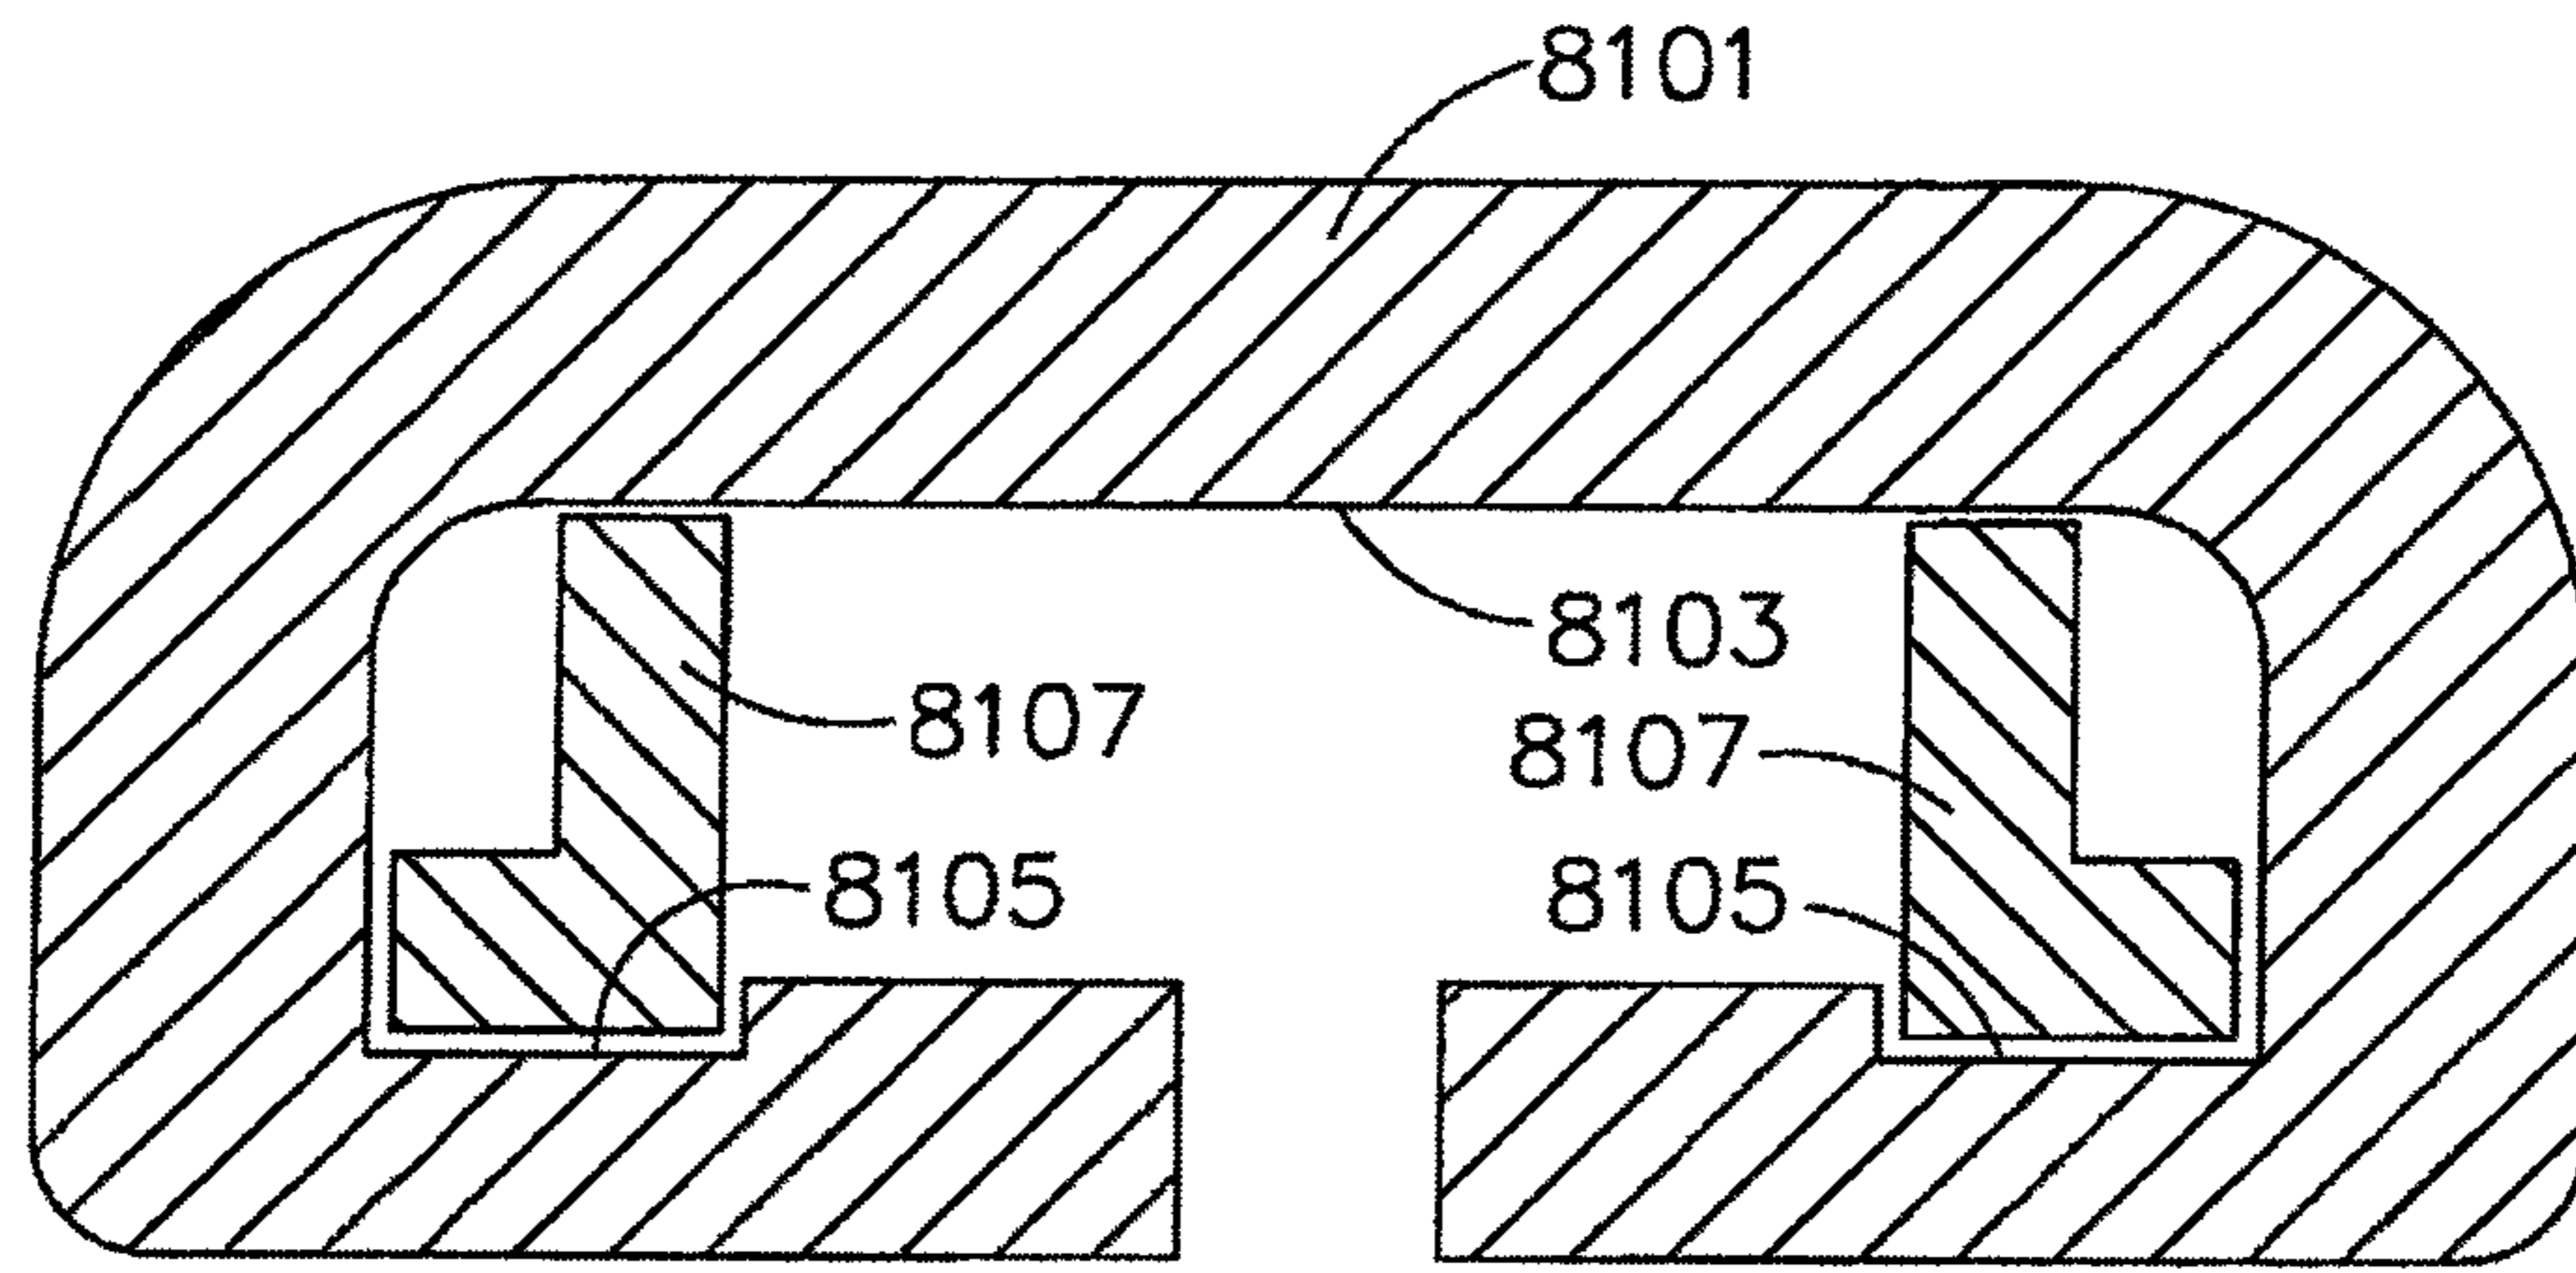


FIG. 100

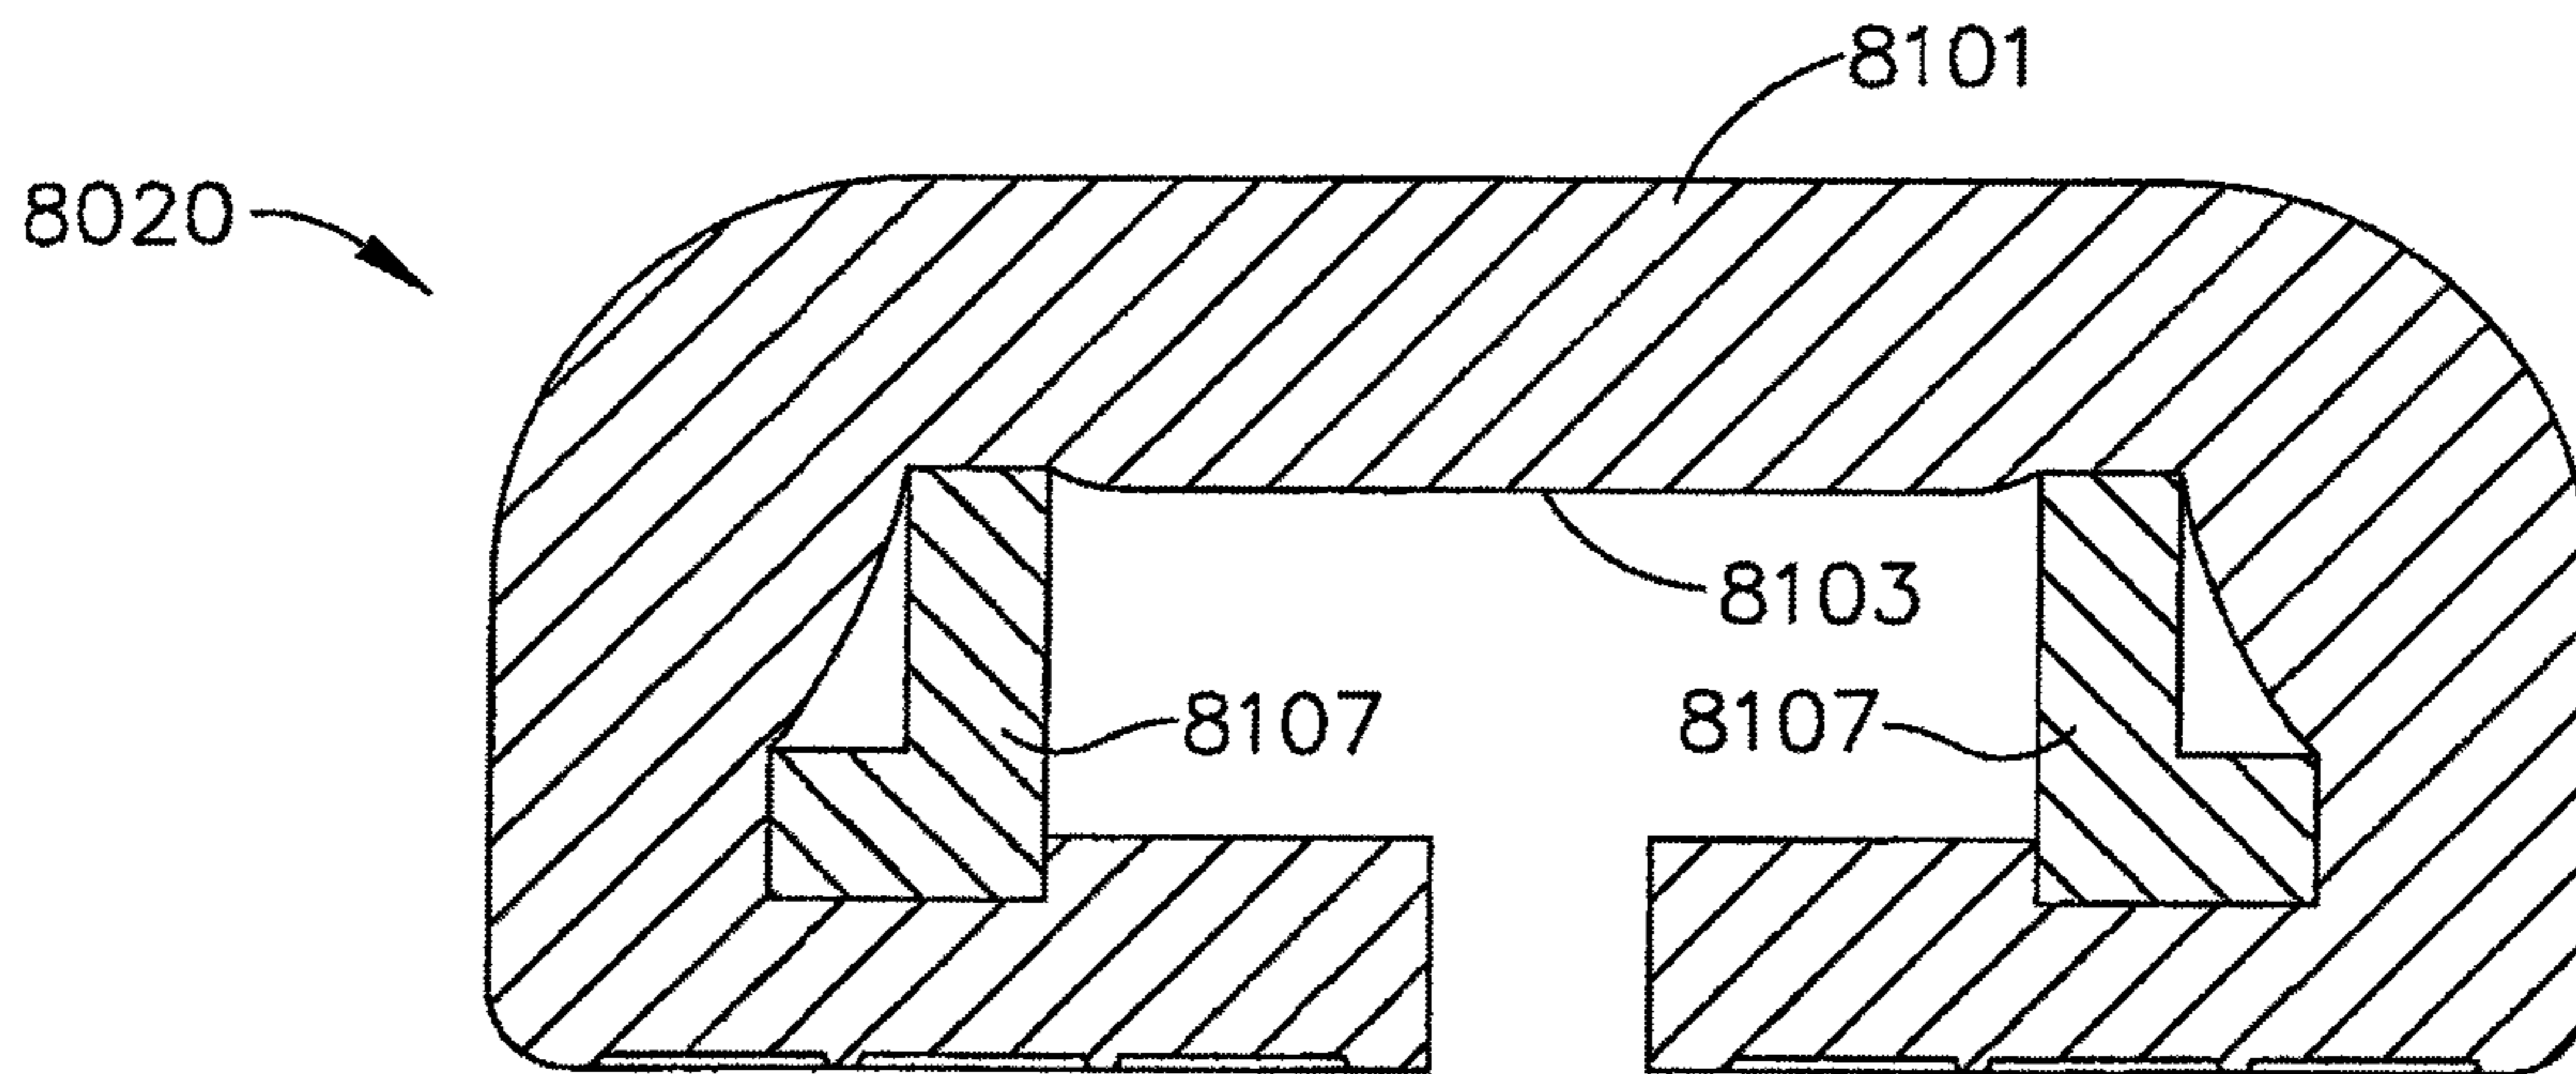


FIG. 101

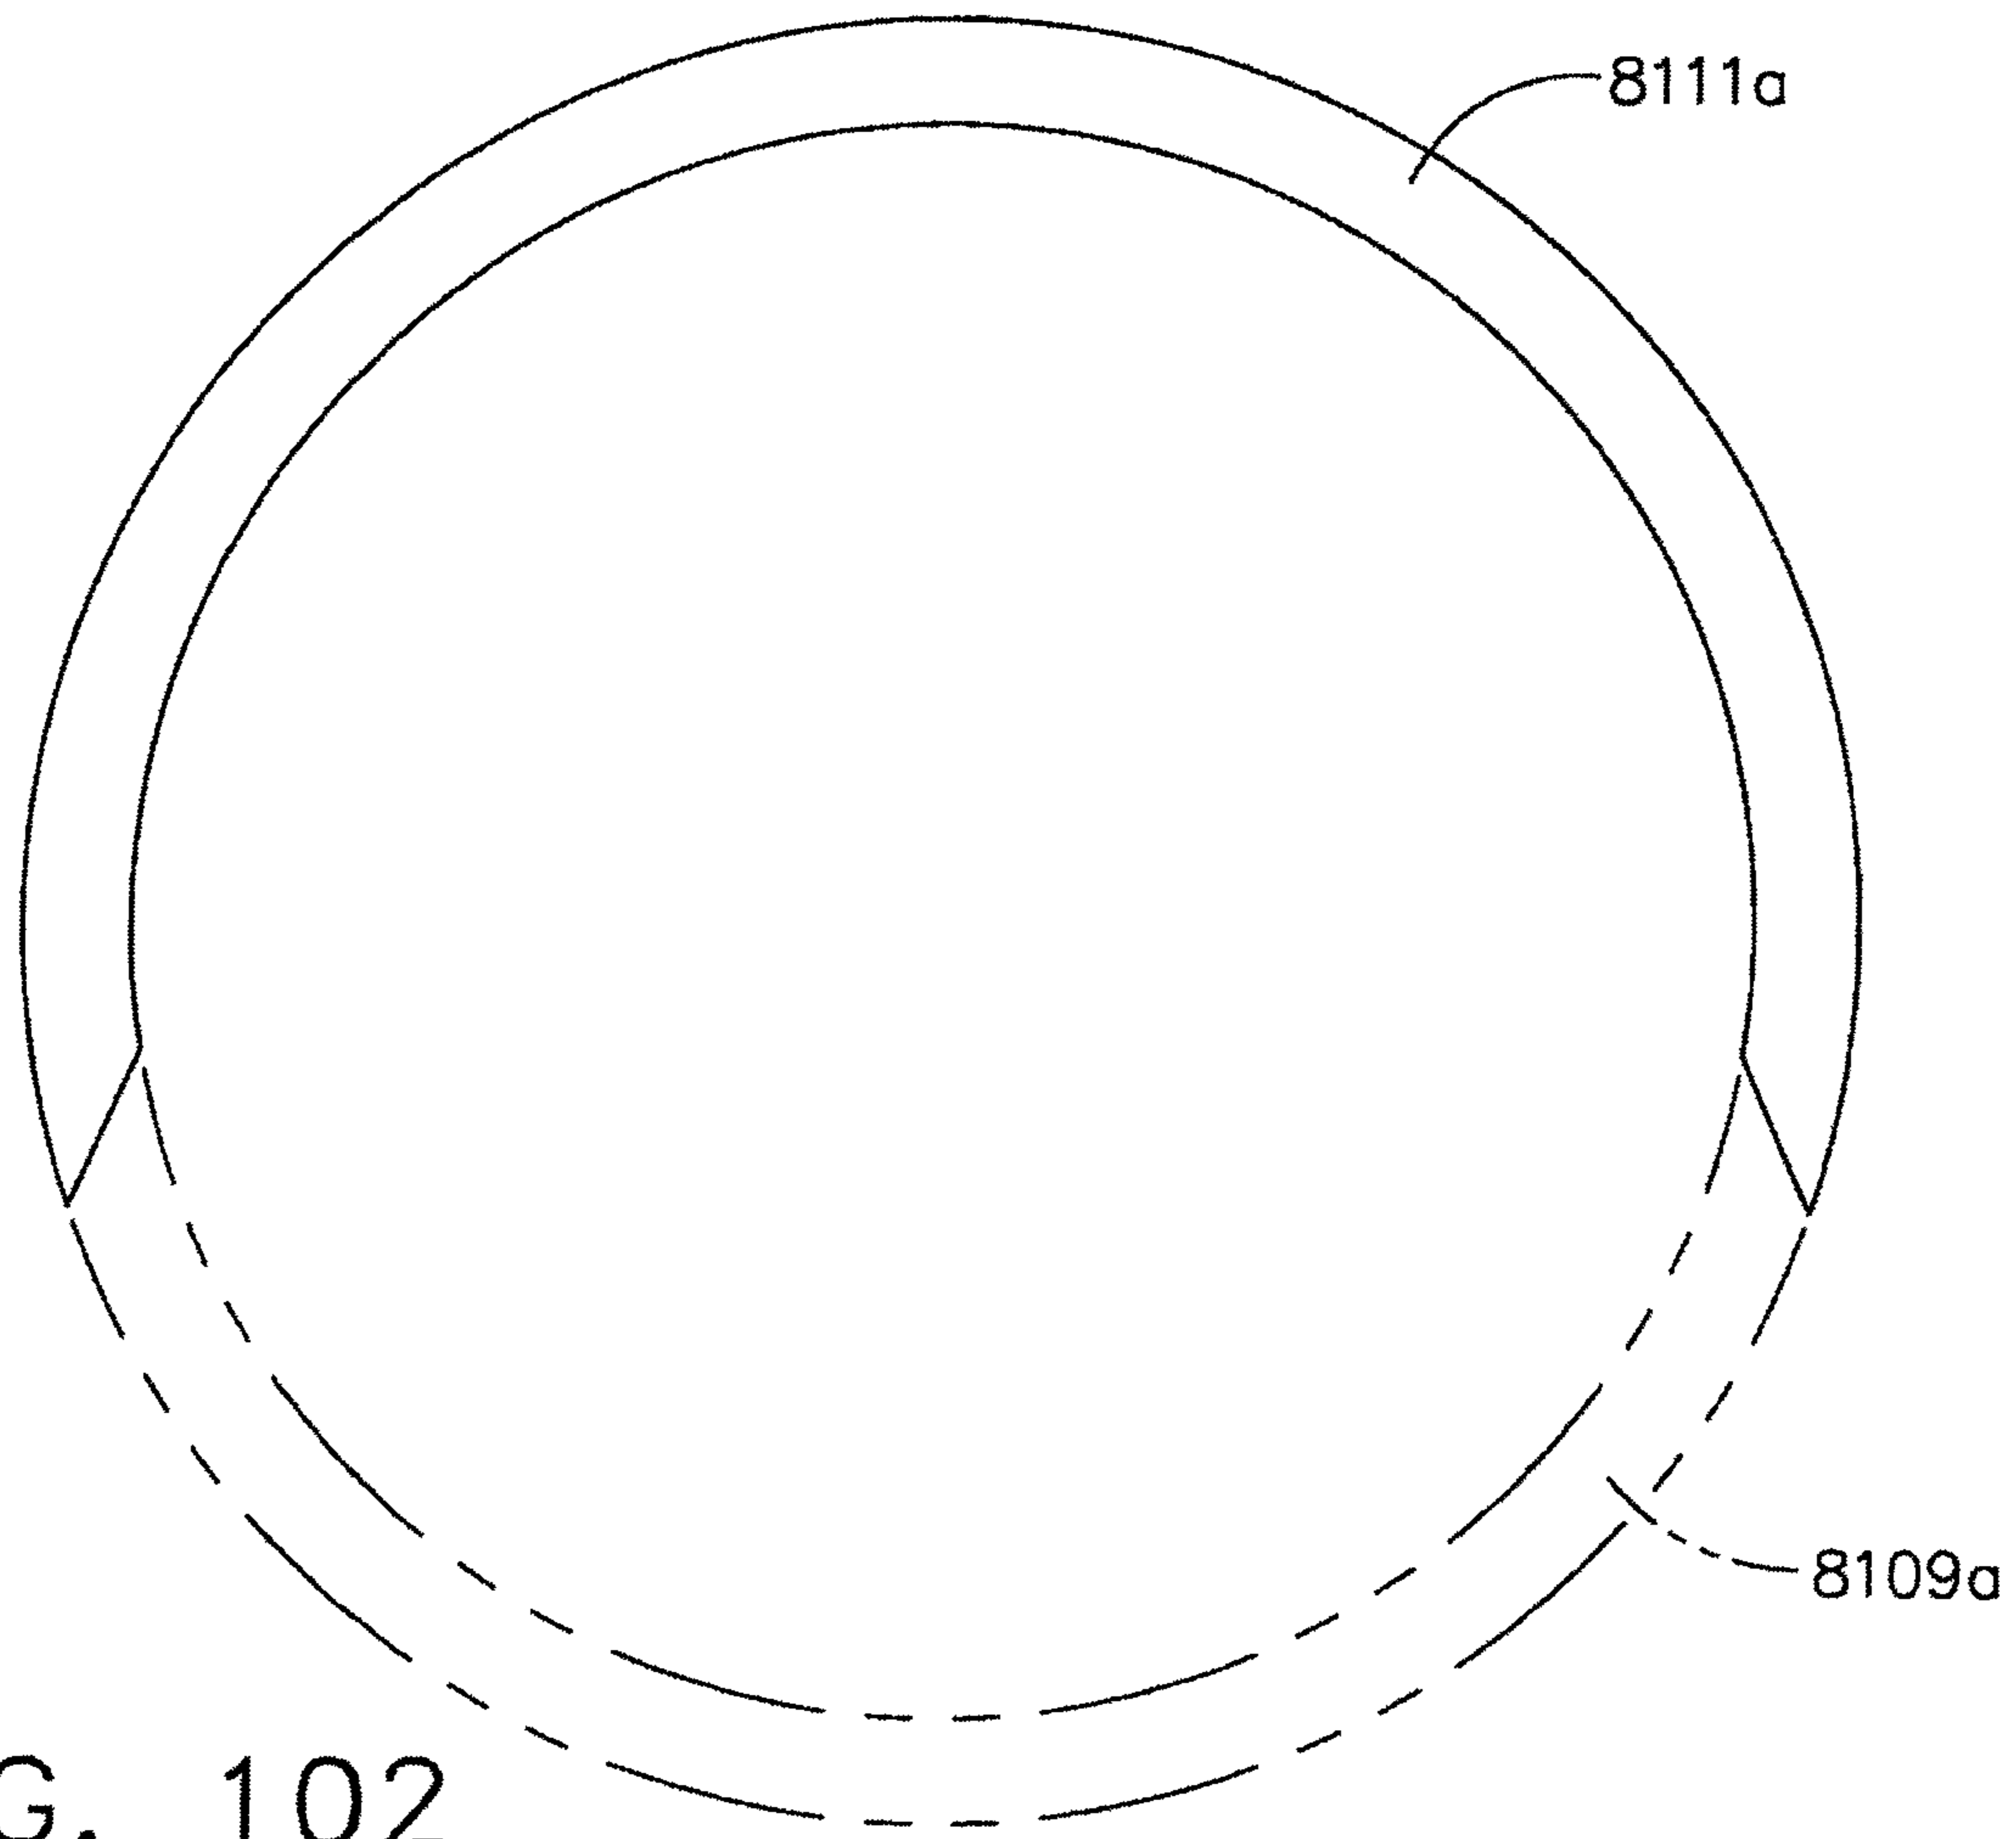


FIG. 102

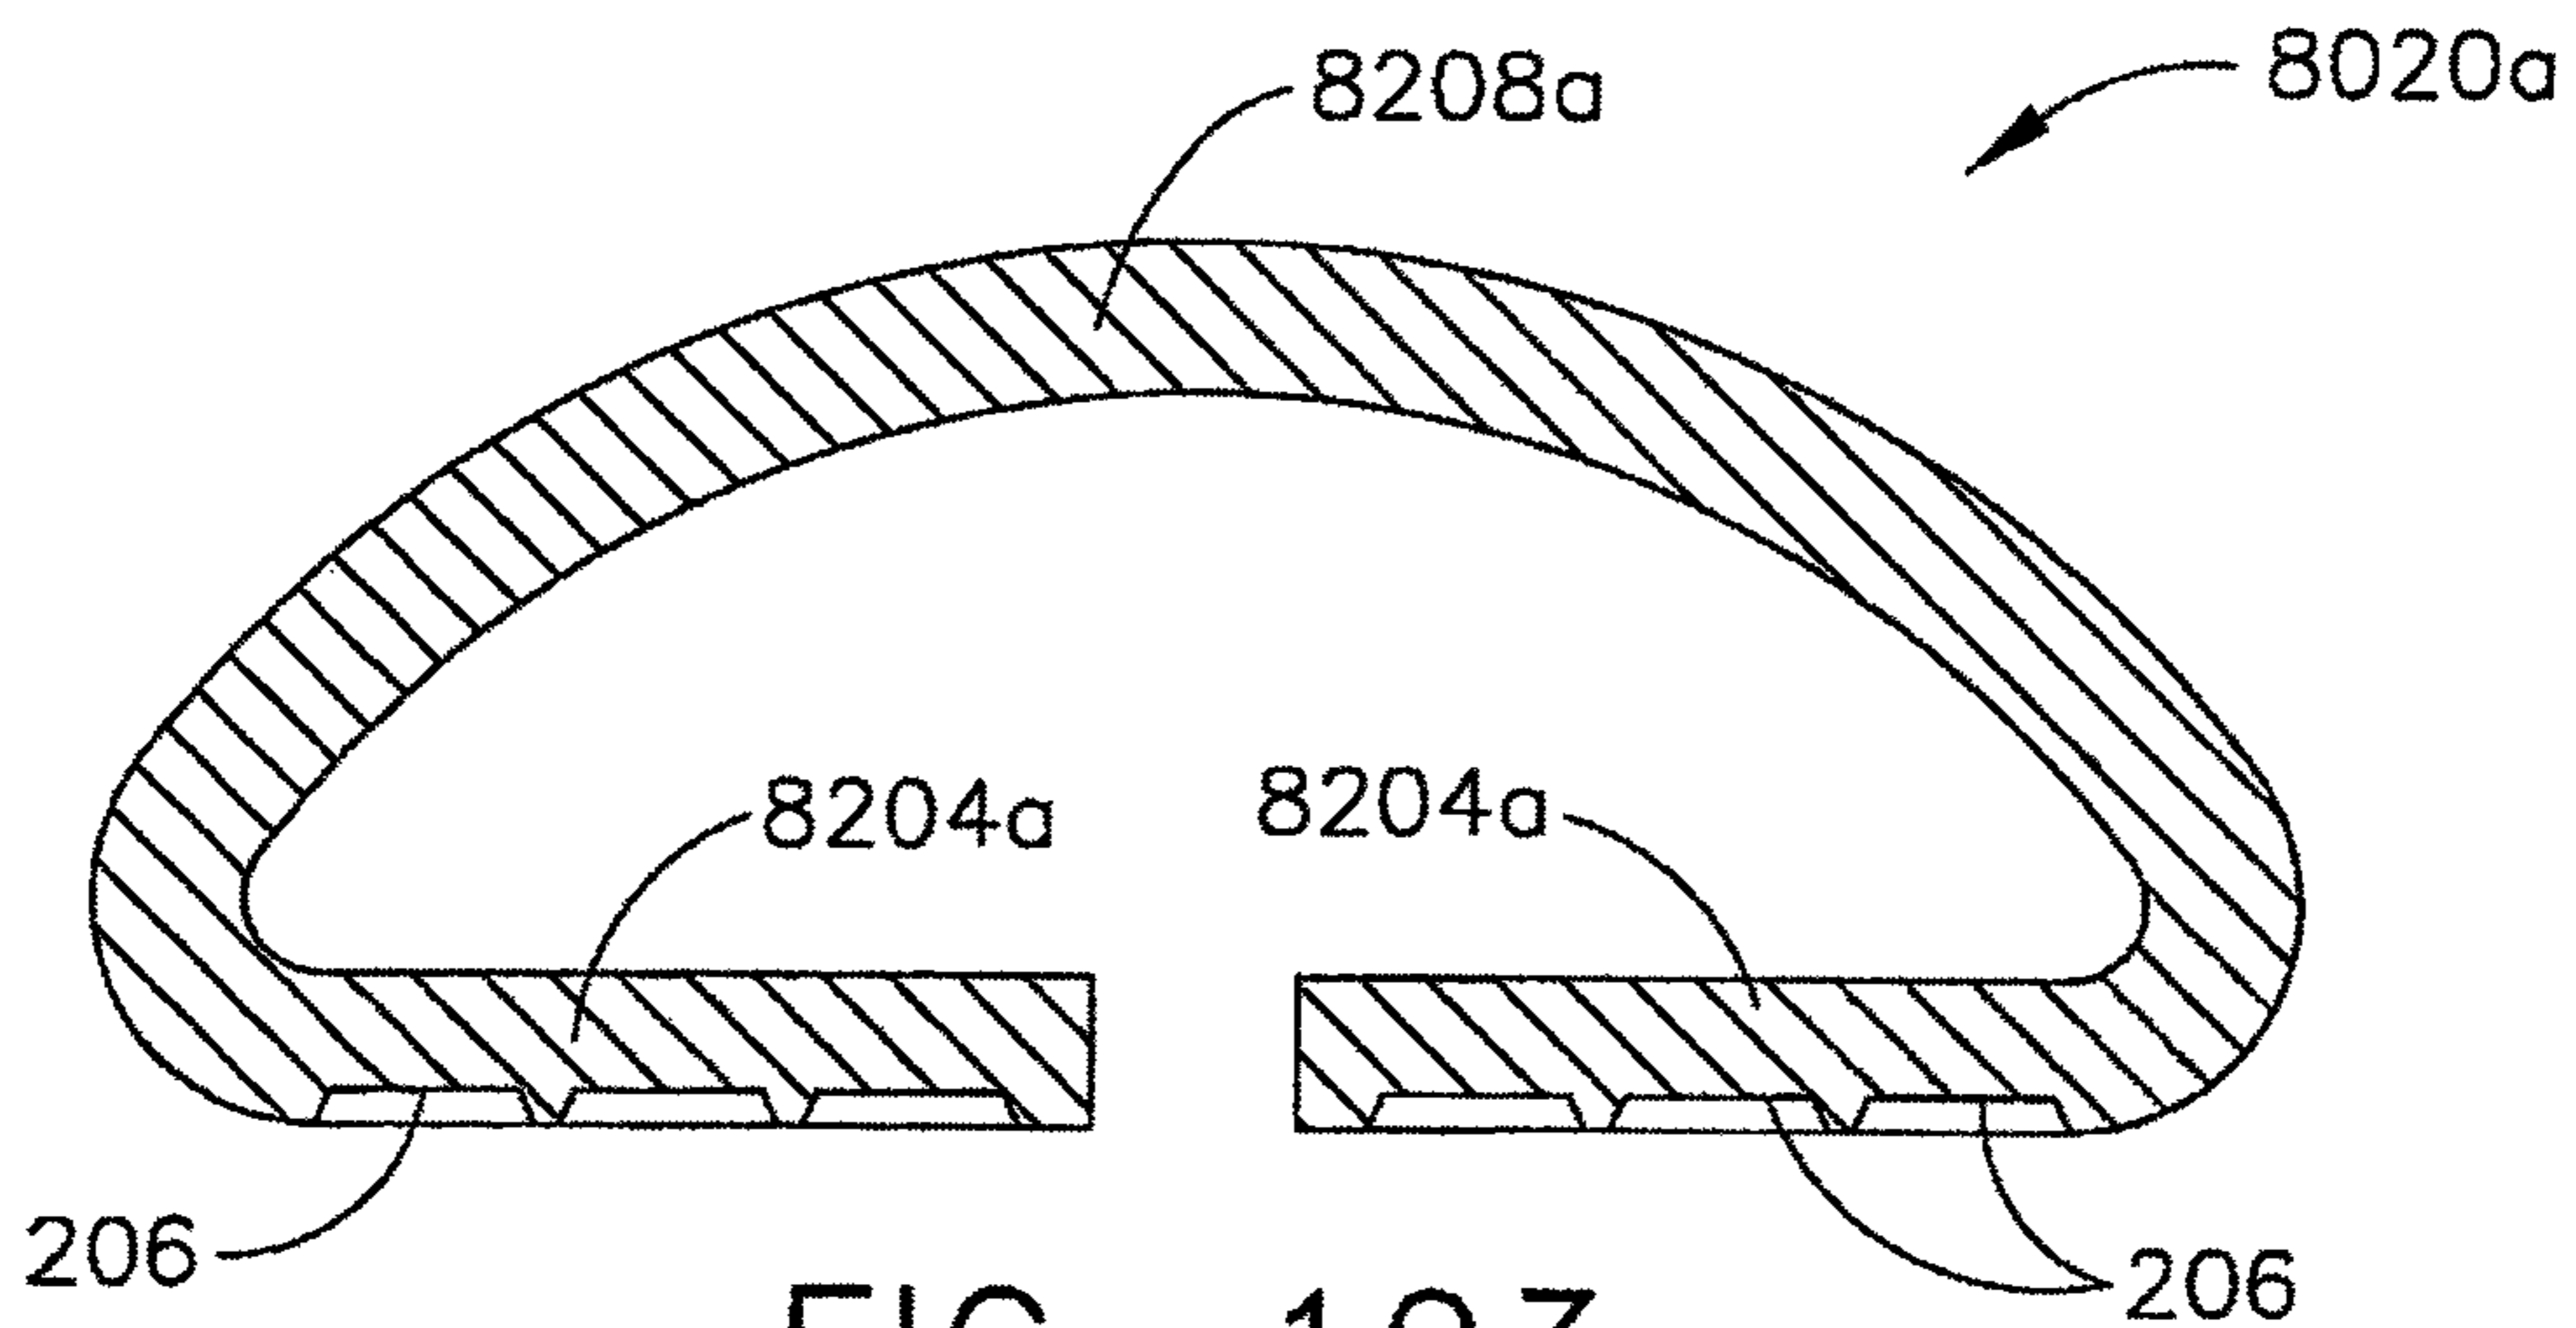


FIG. 103

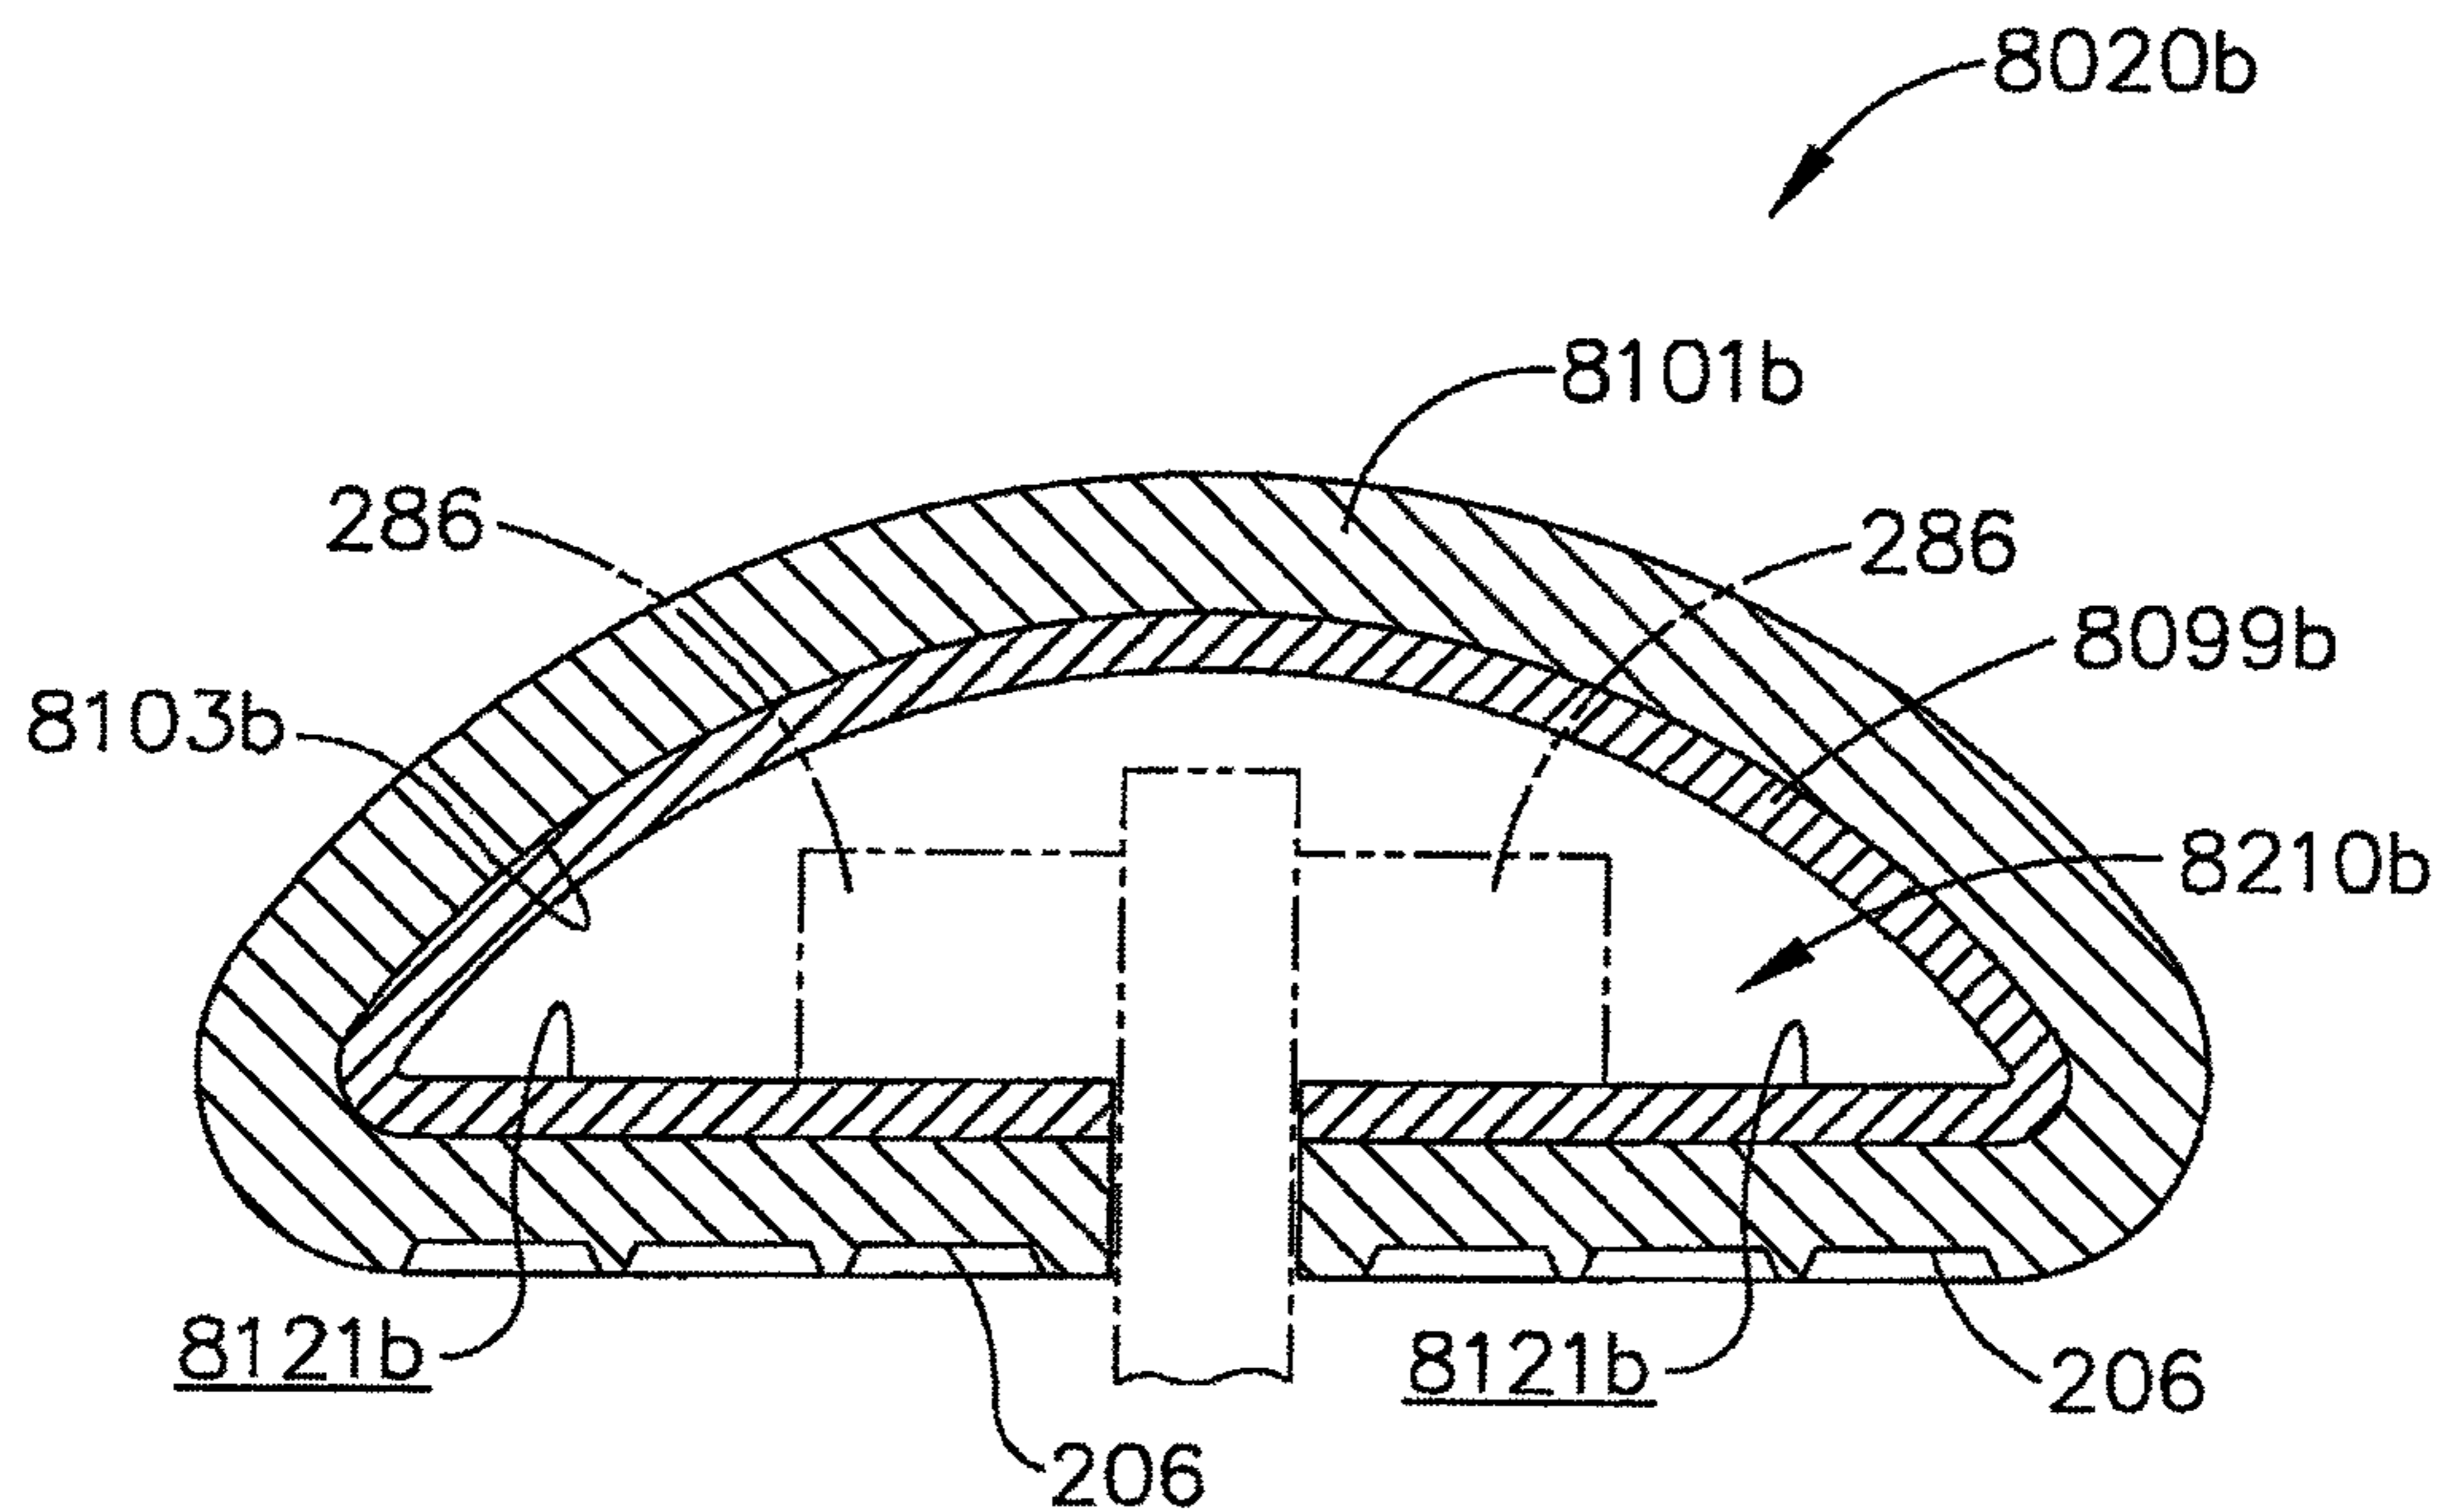


FIG. 104

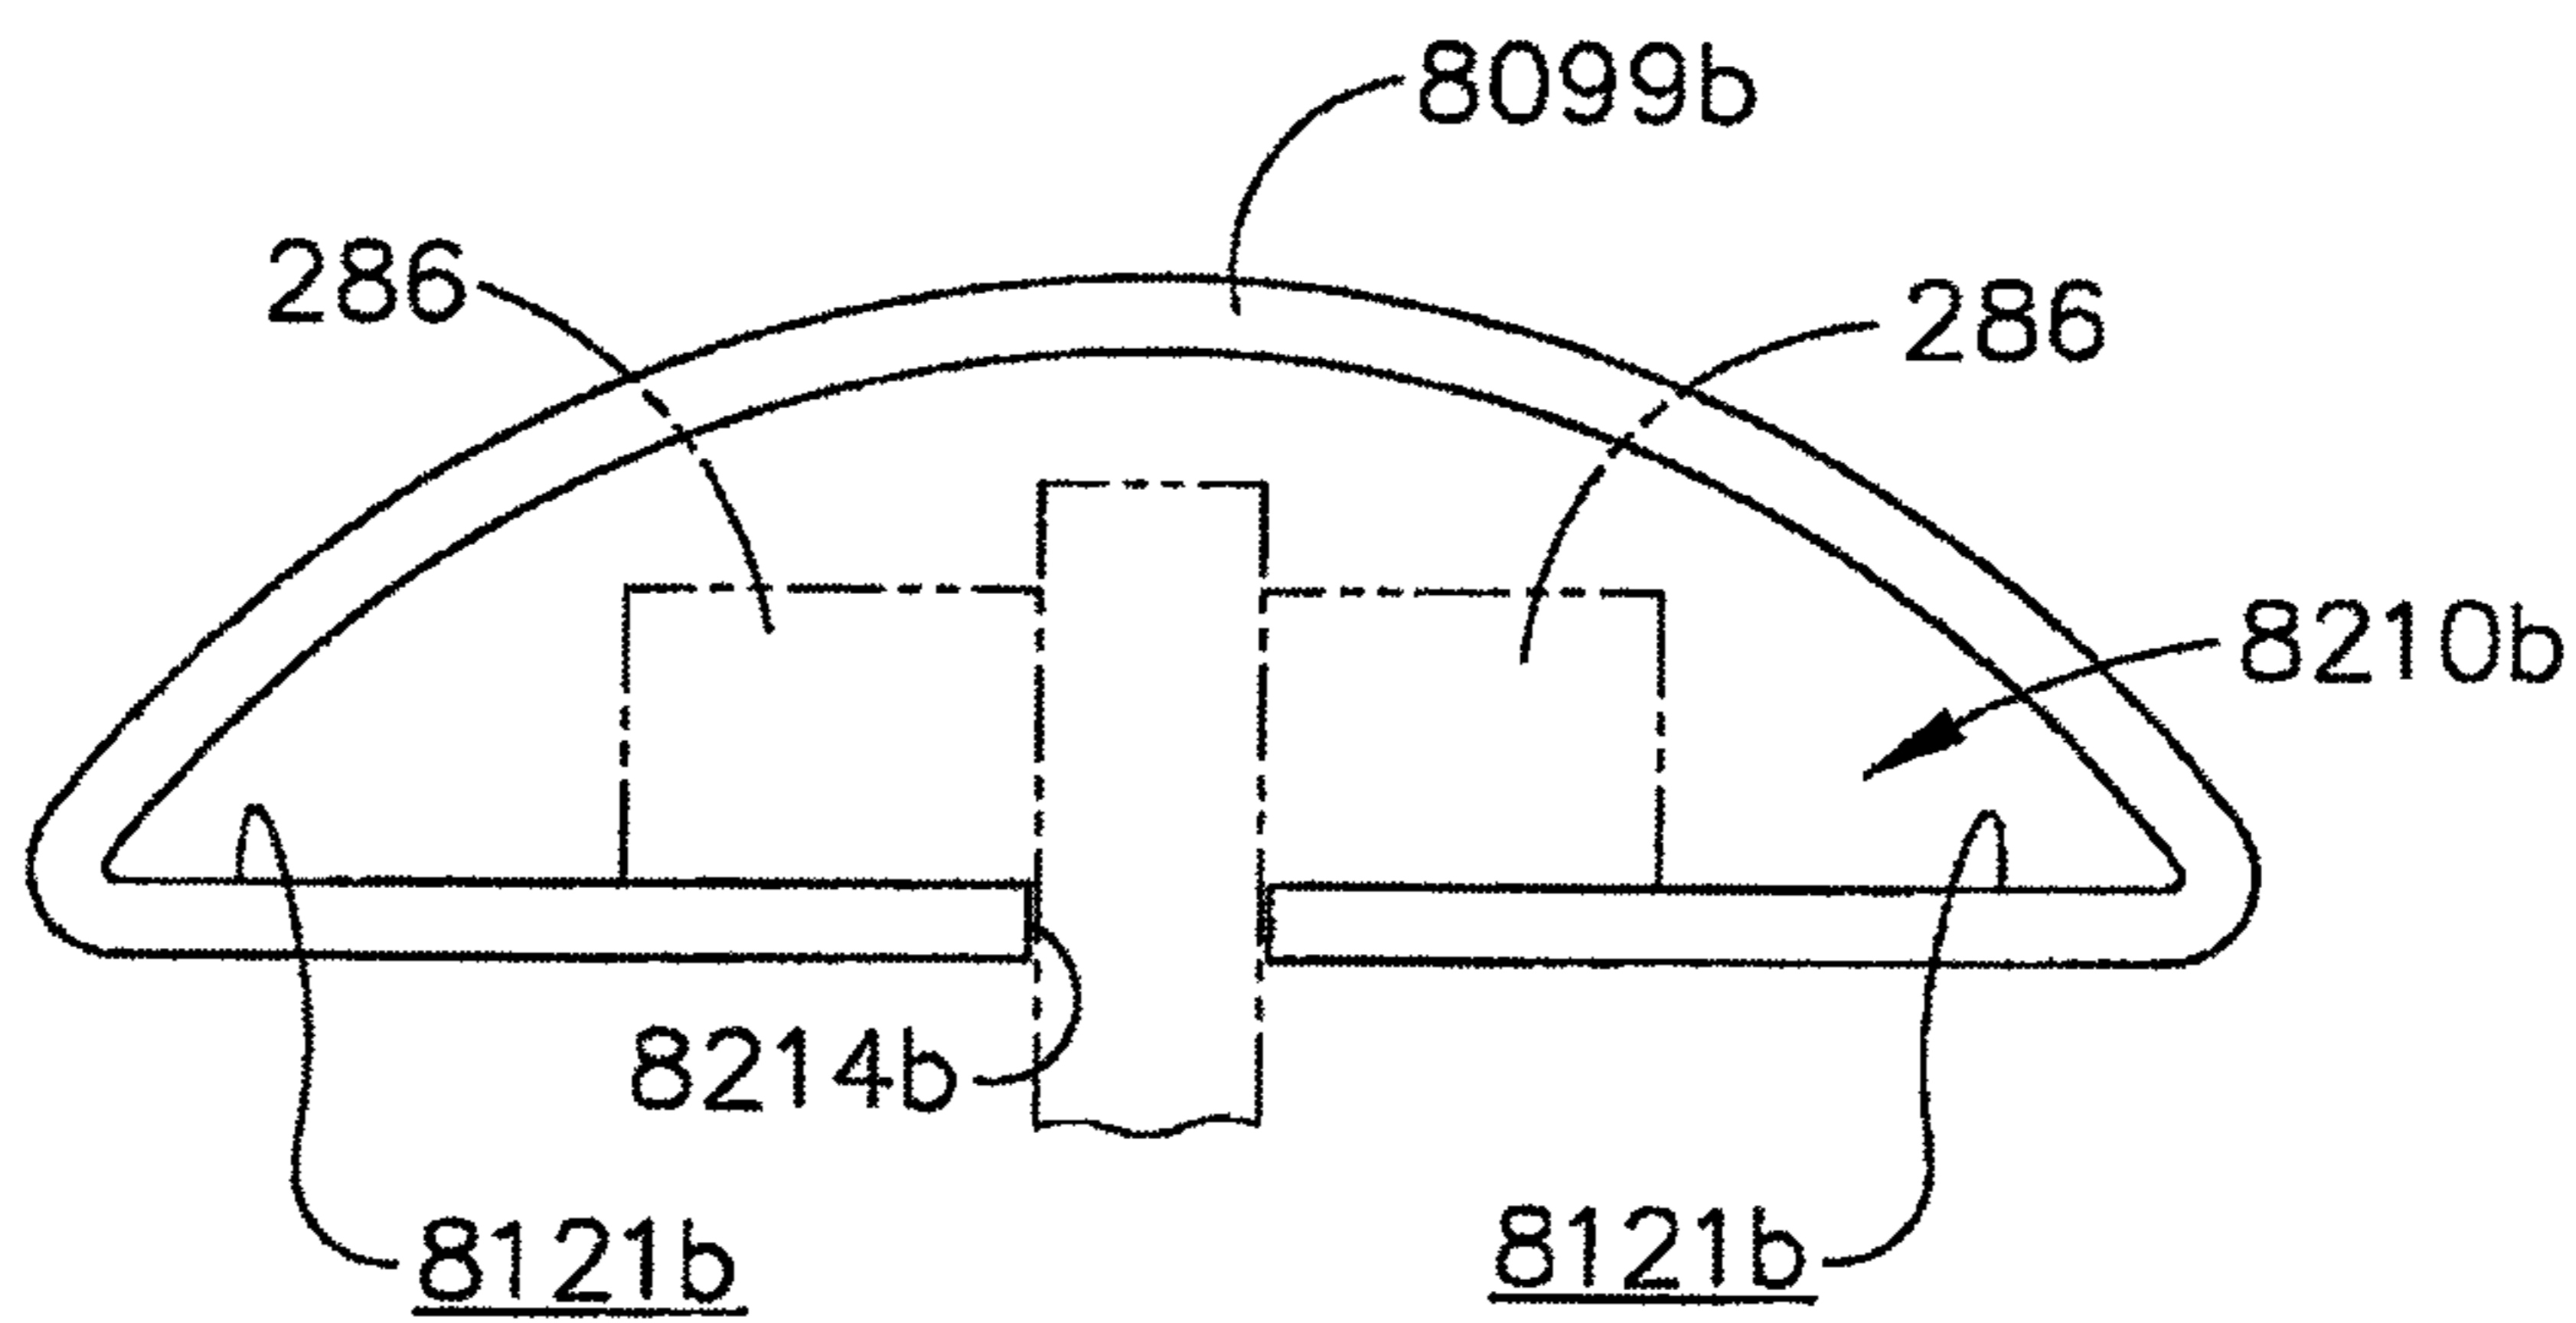


FIG. 105

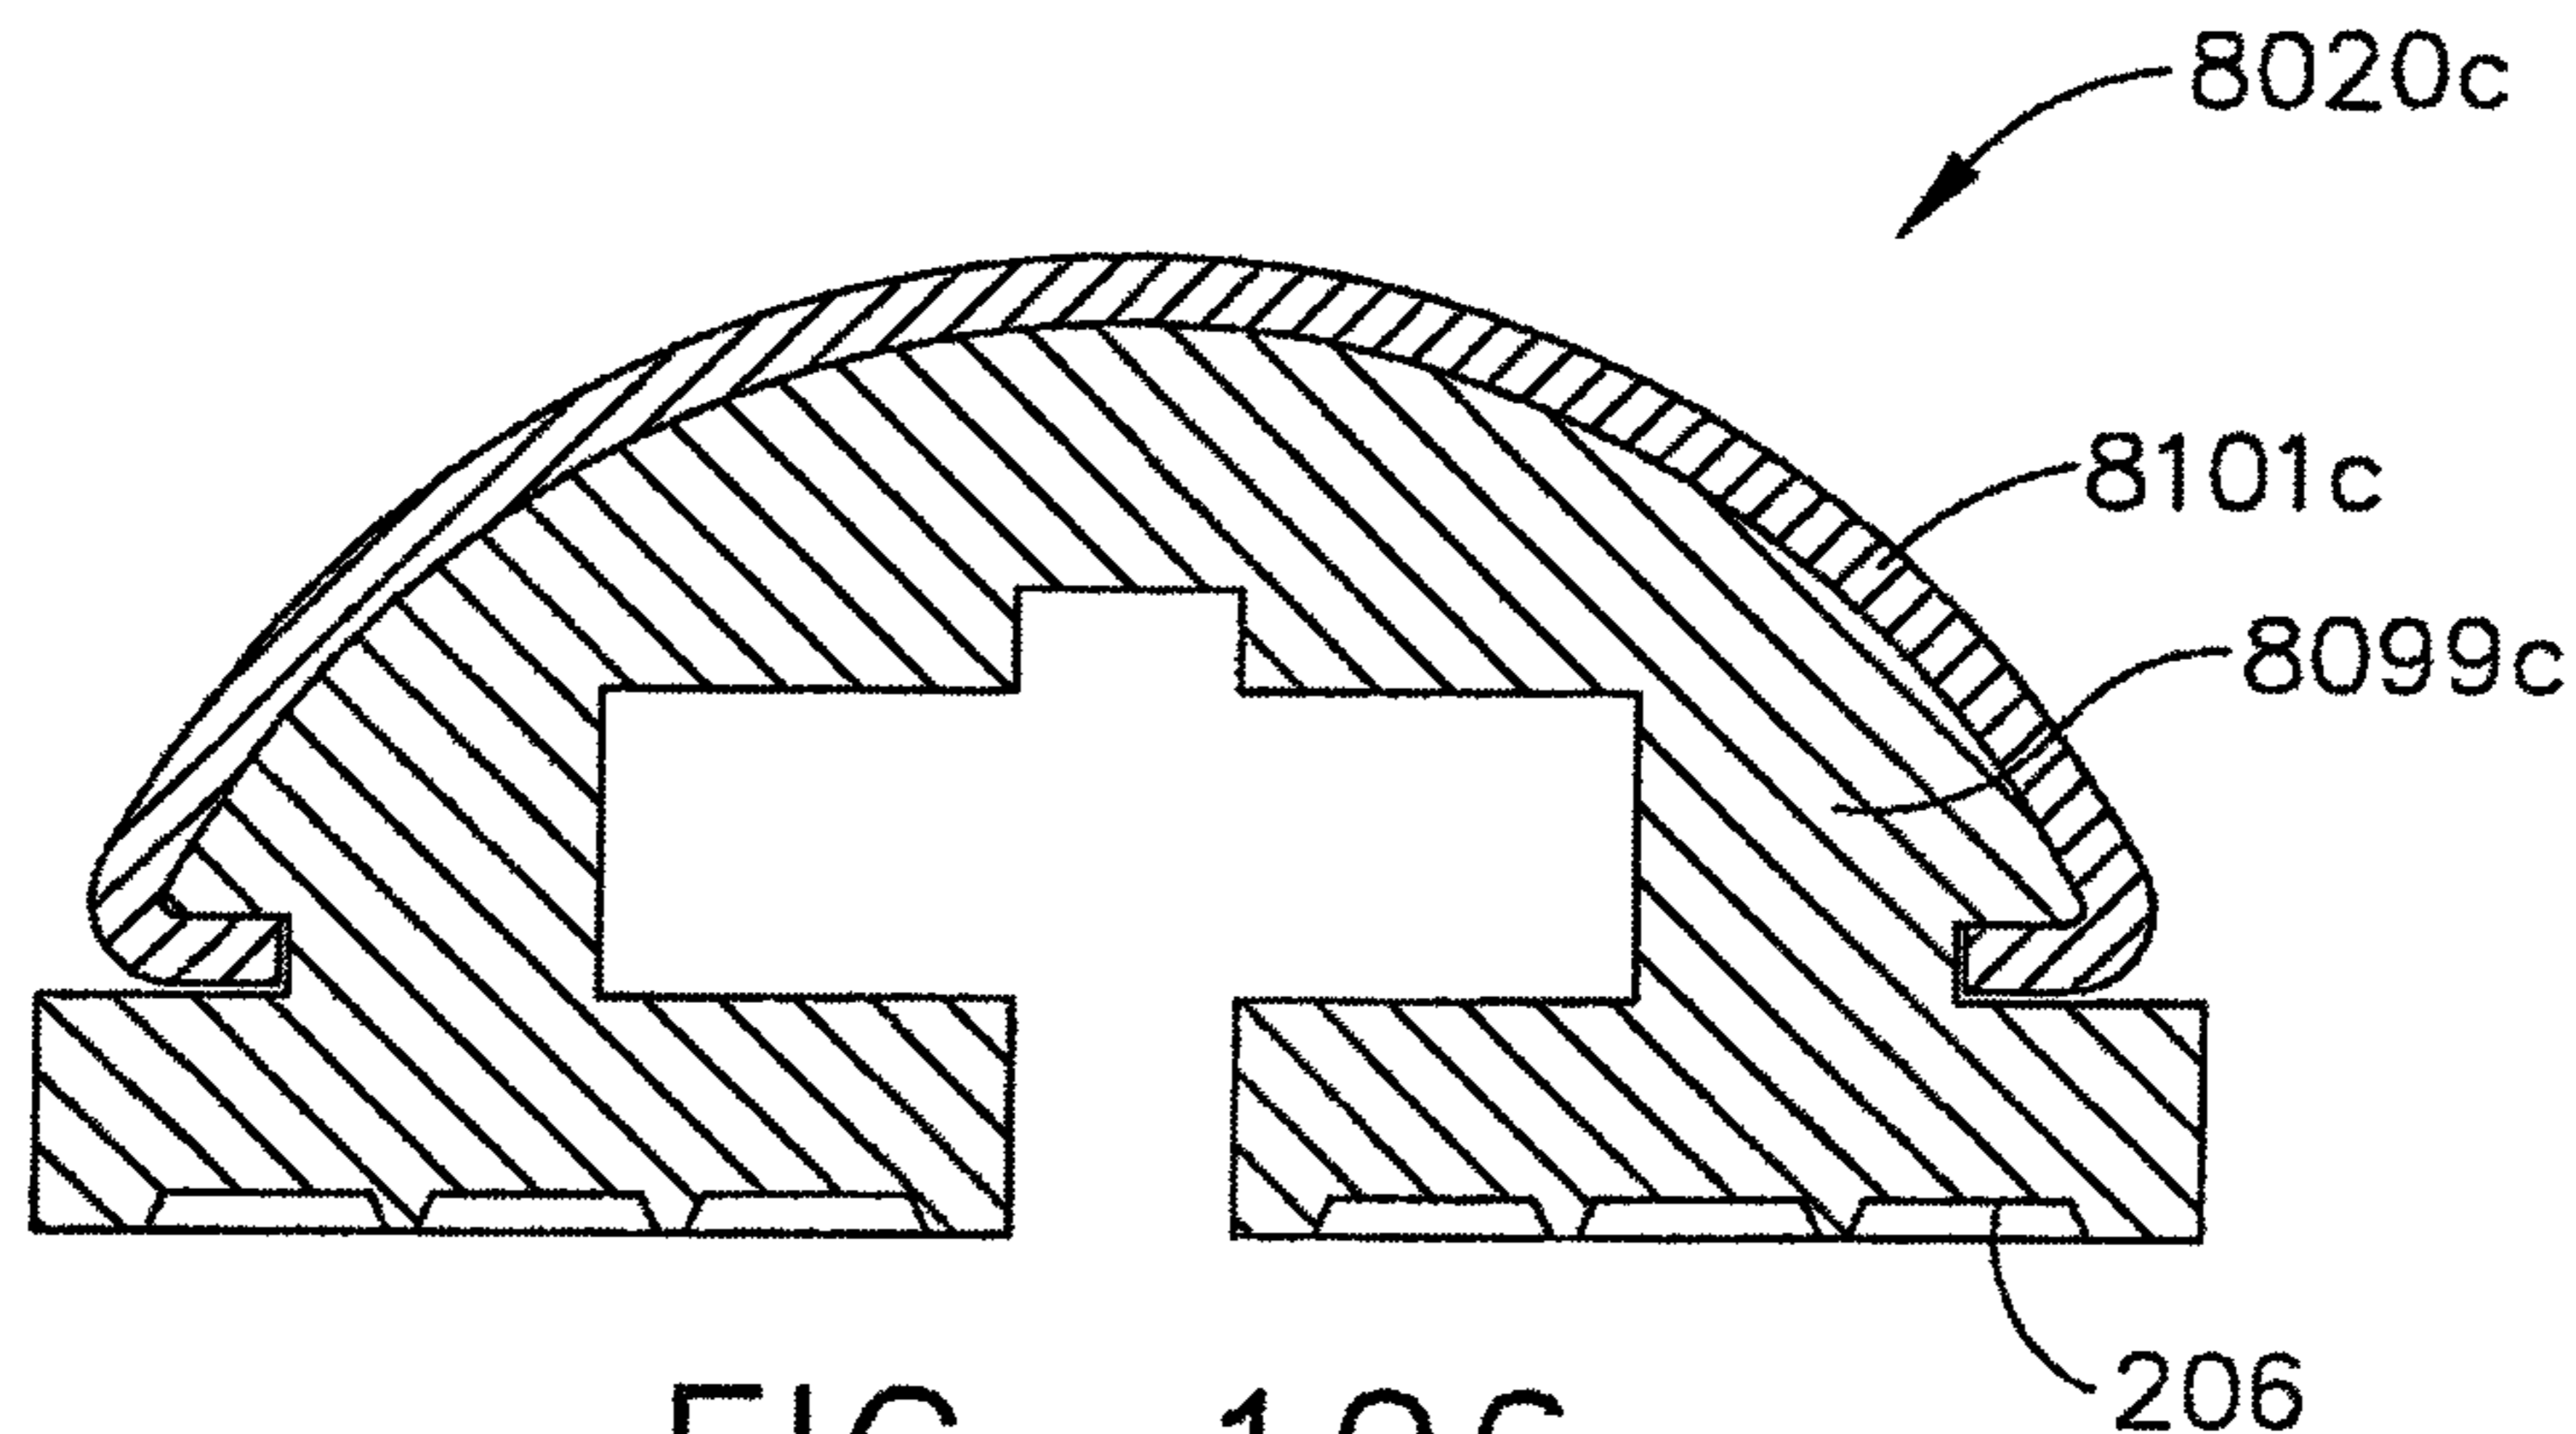


FIG. 106

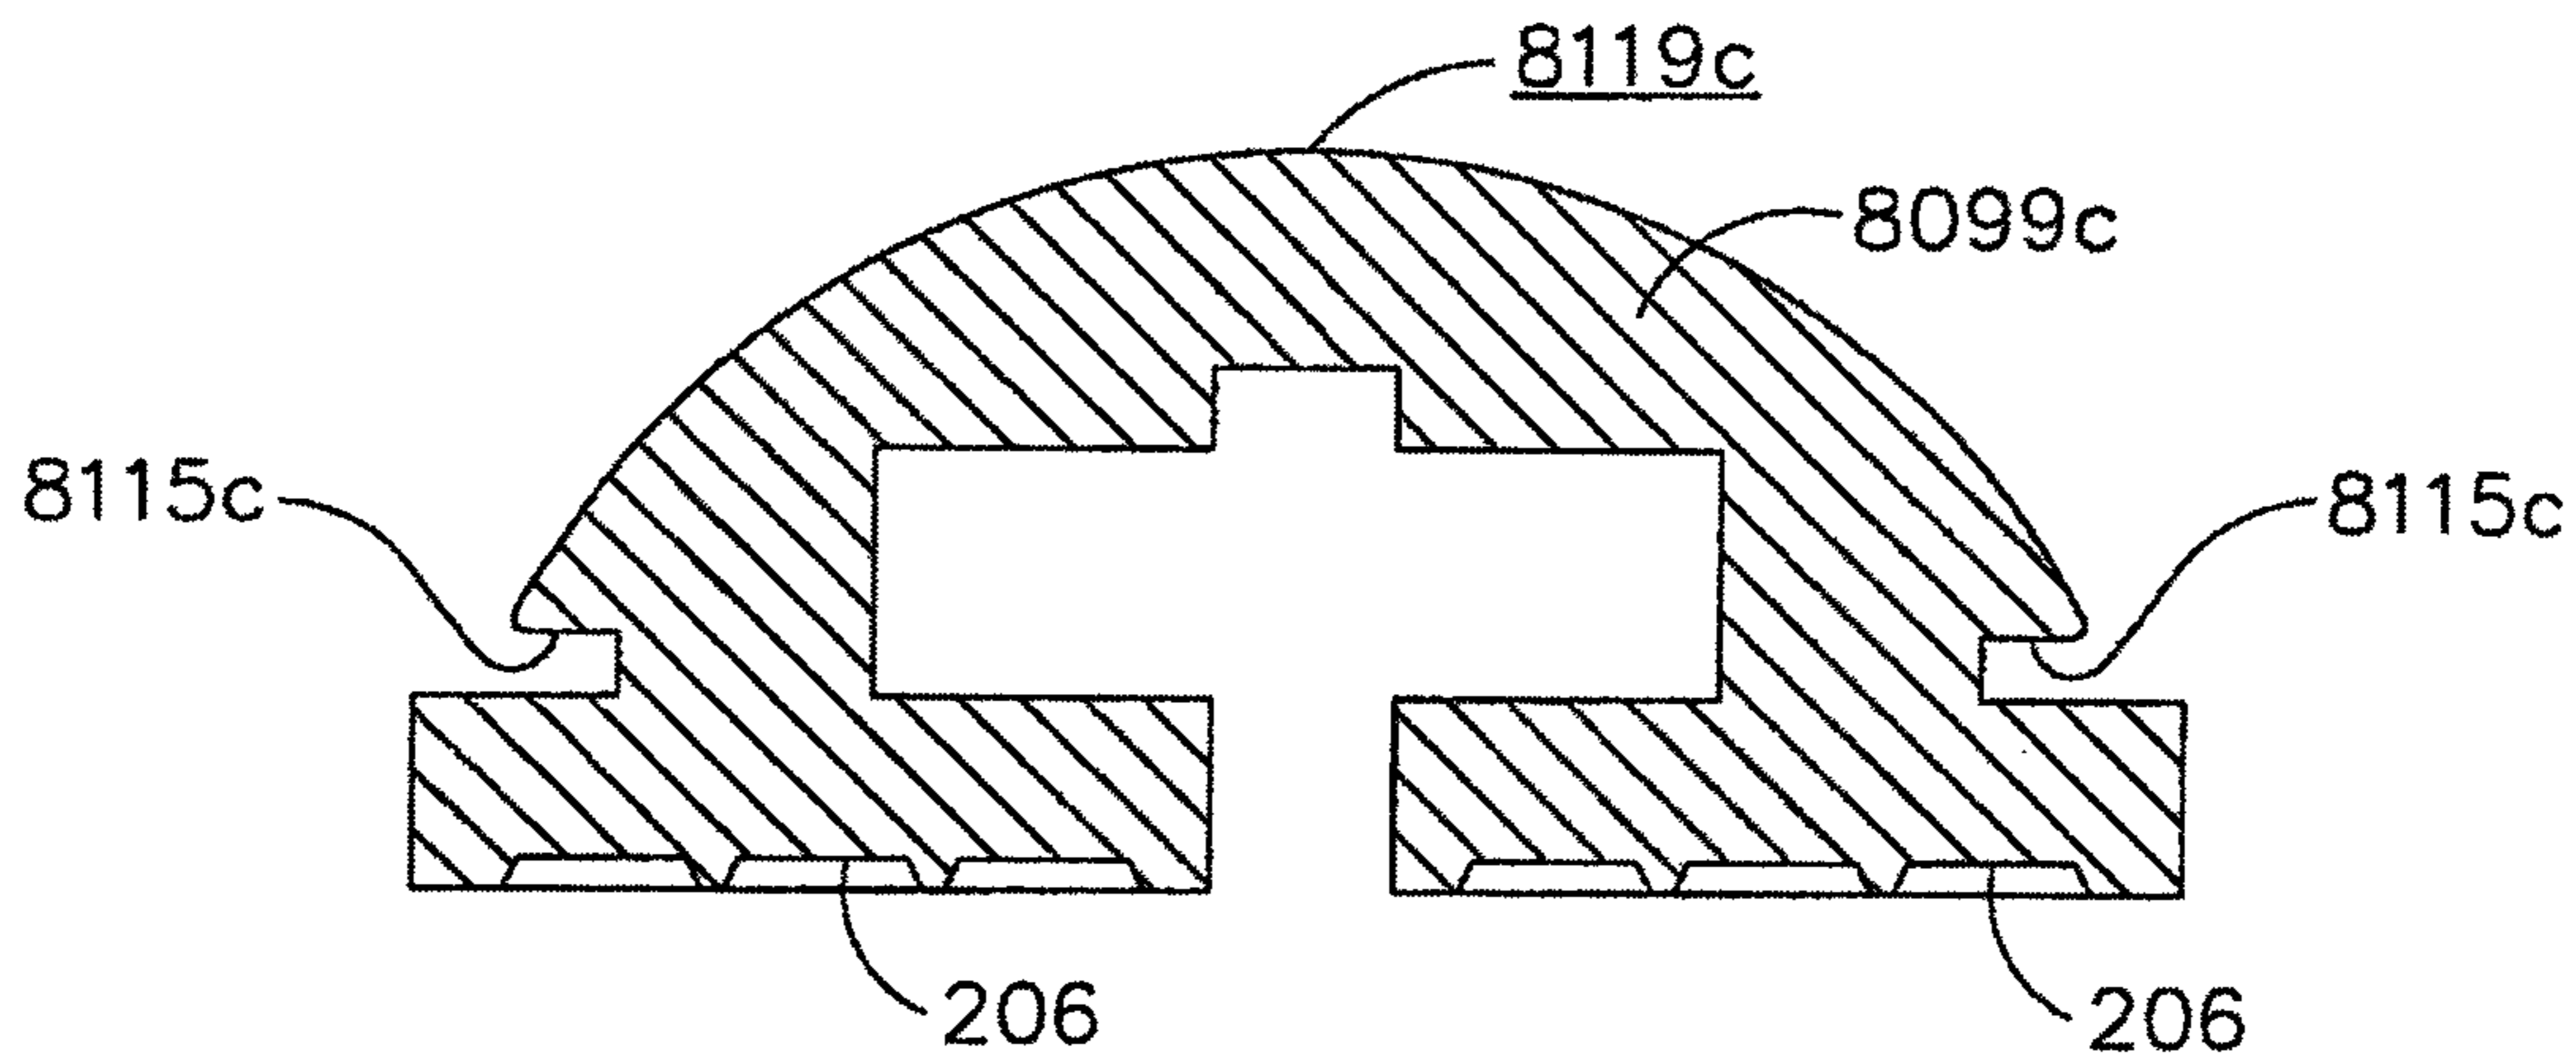


FIG. 107

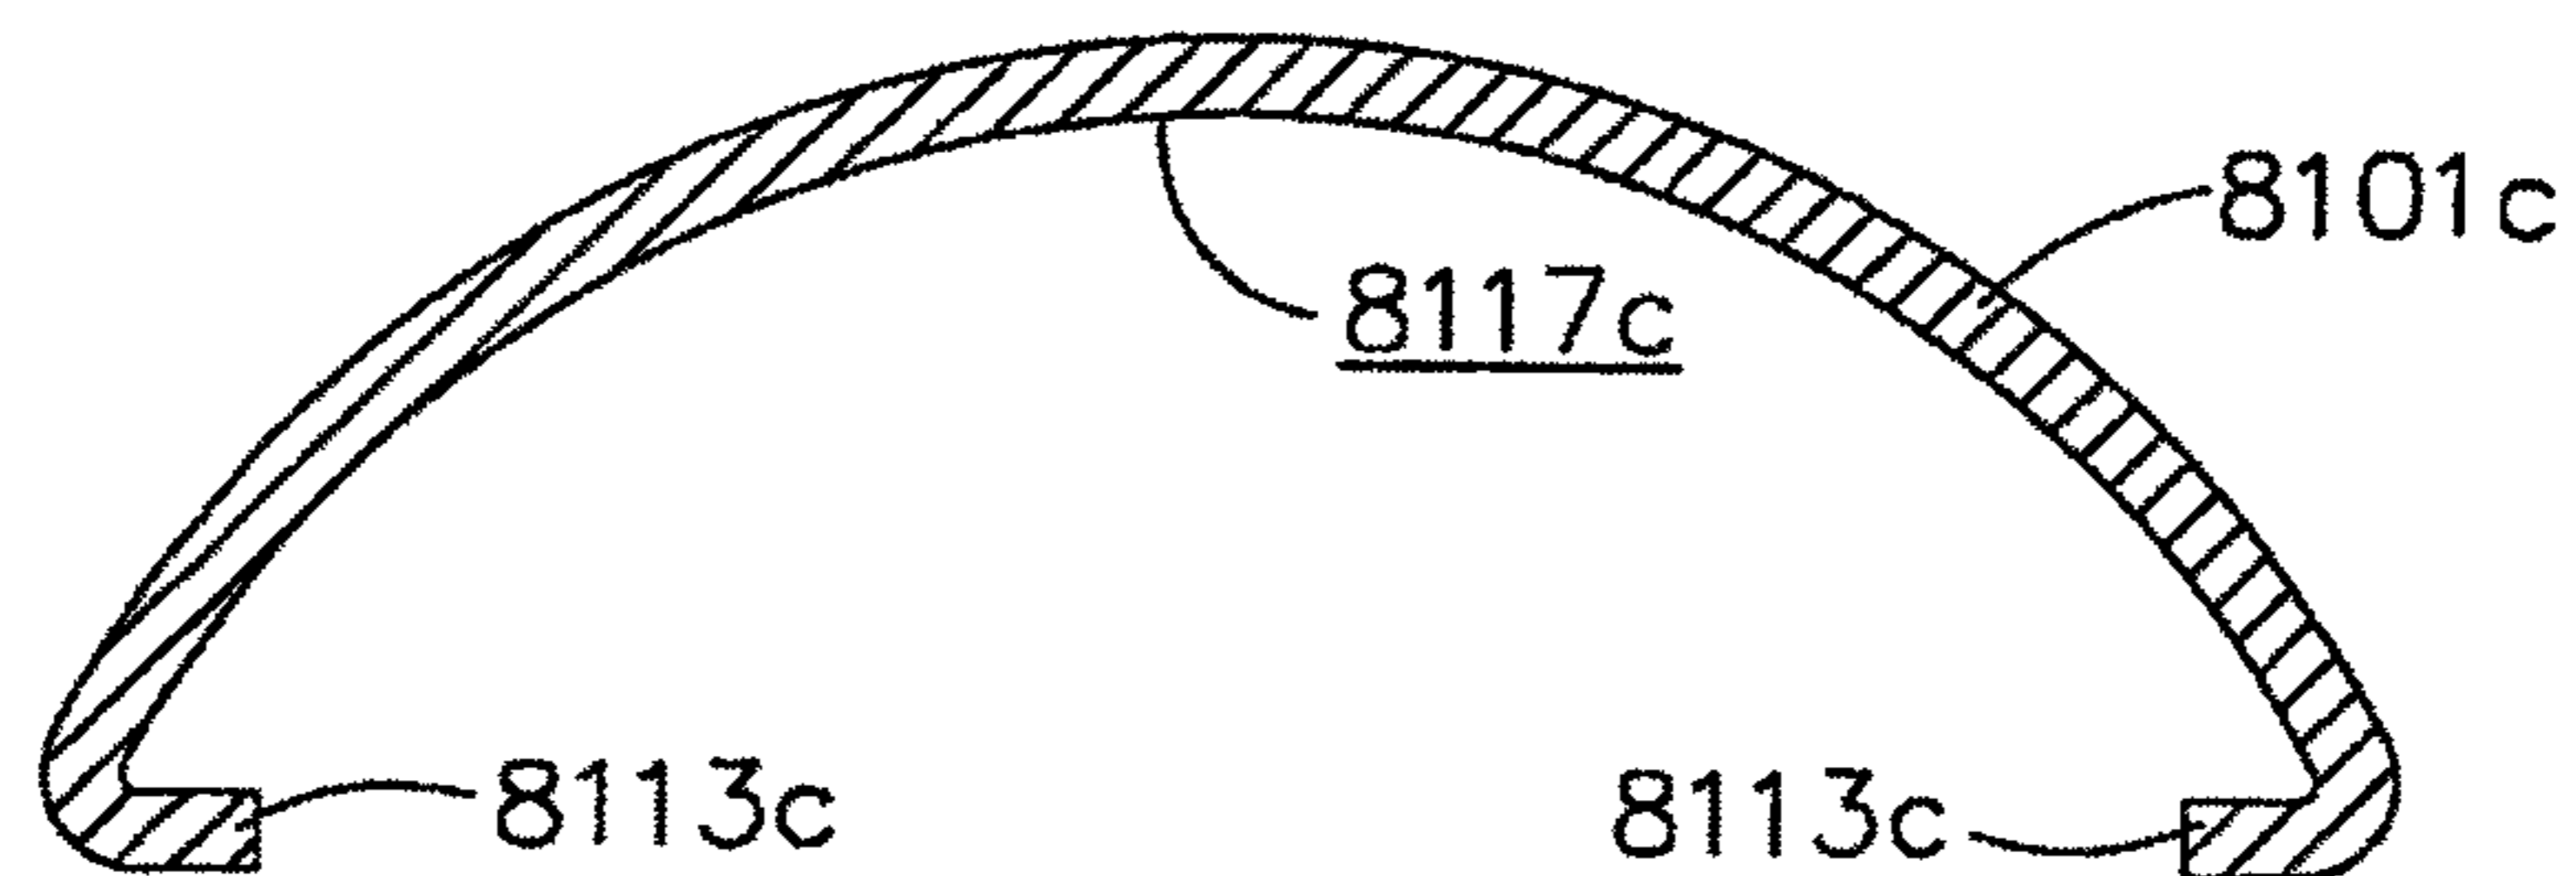


FIG. 108

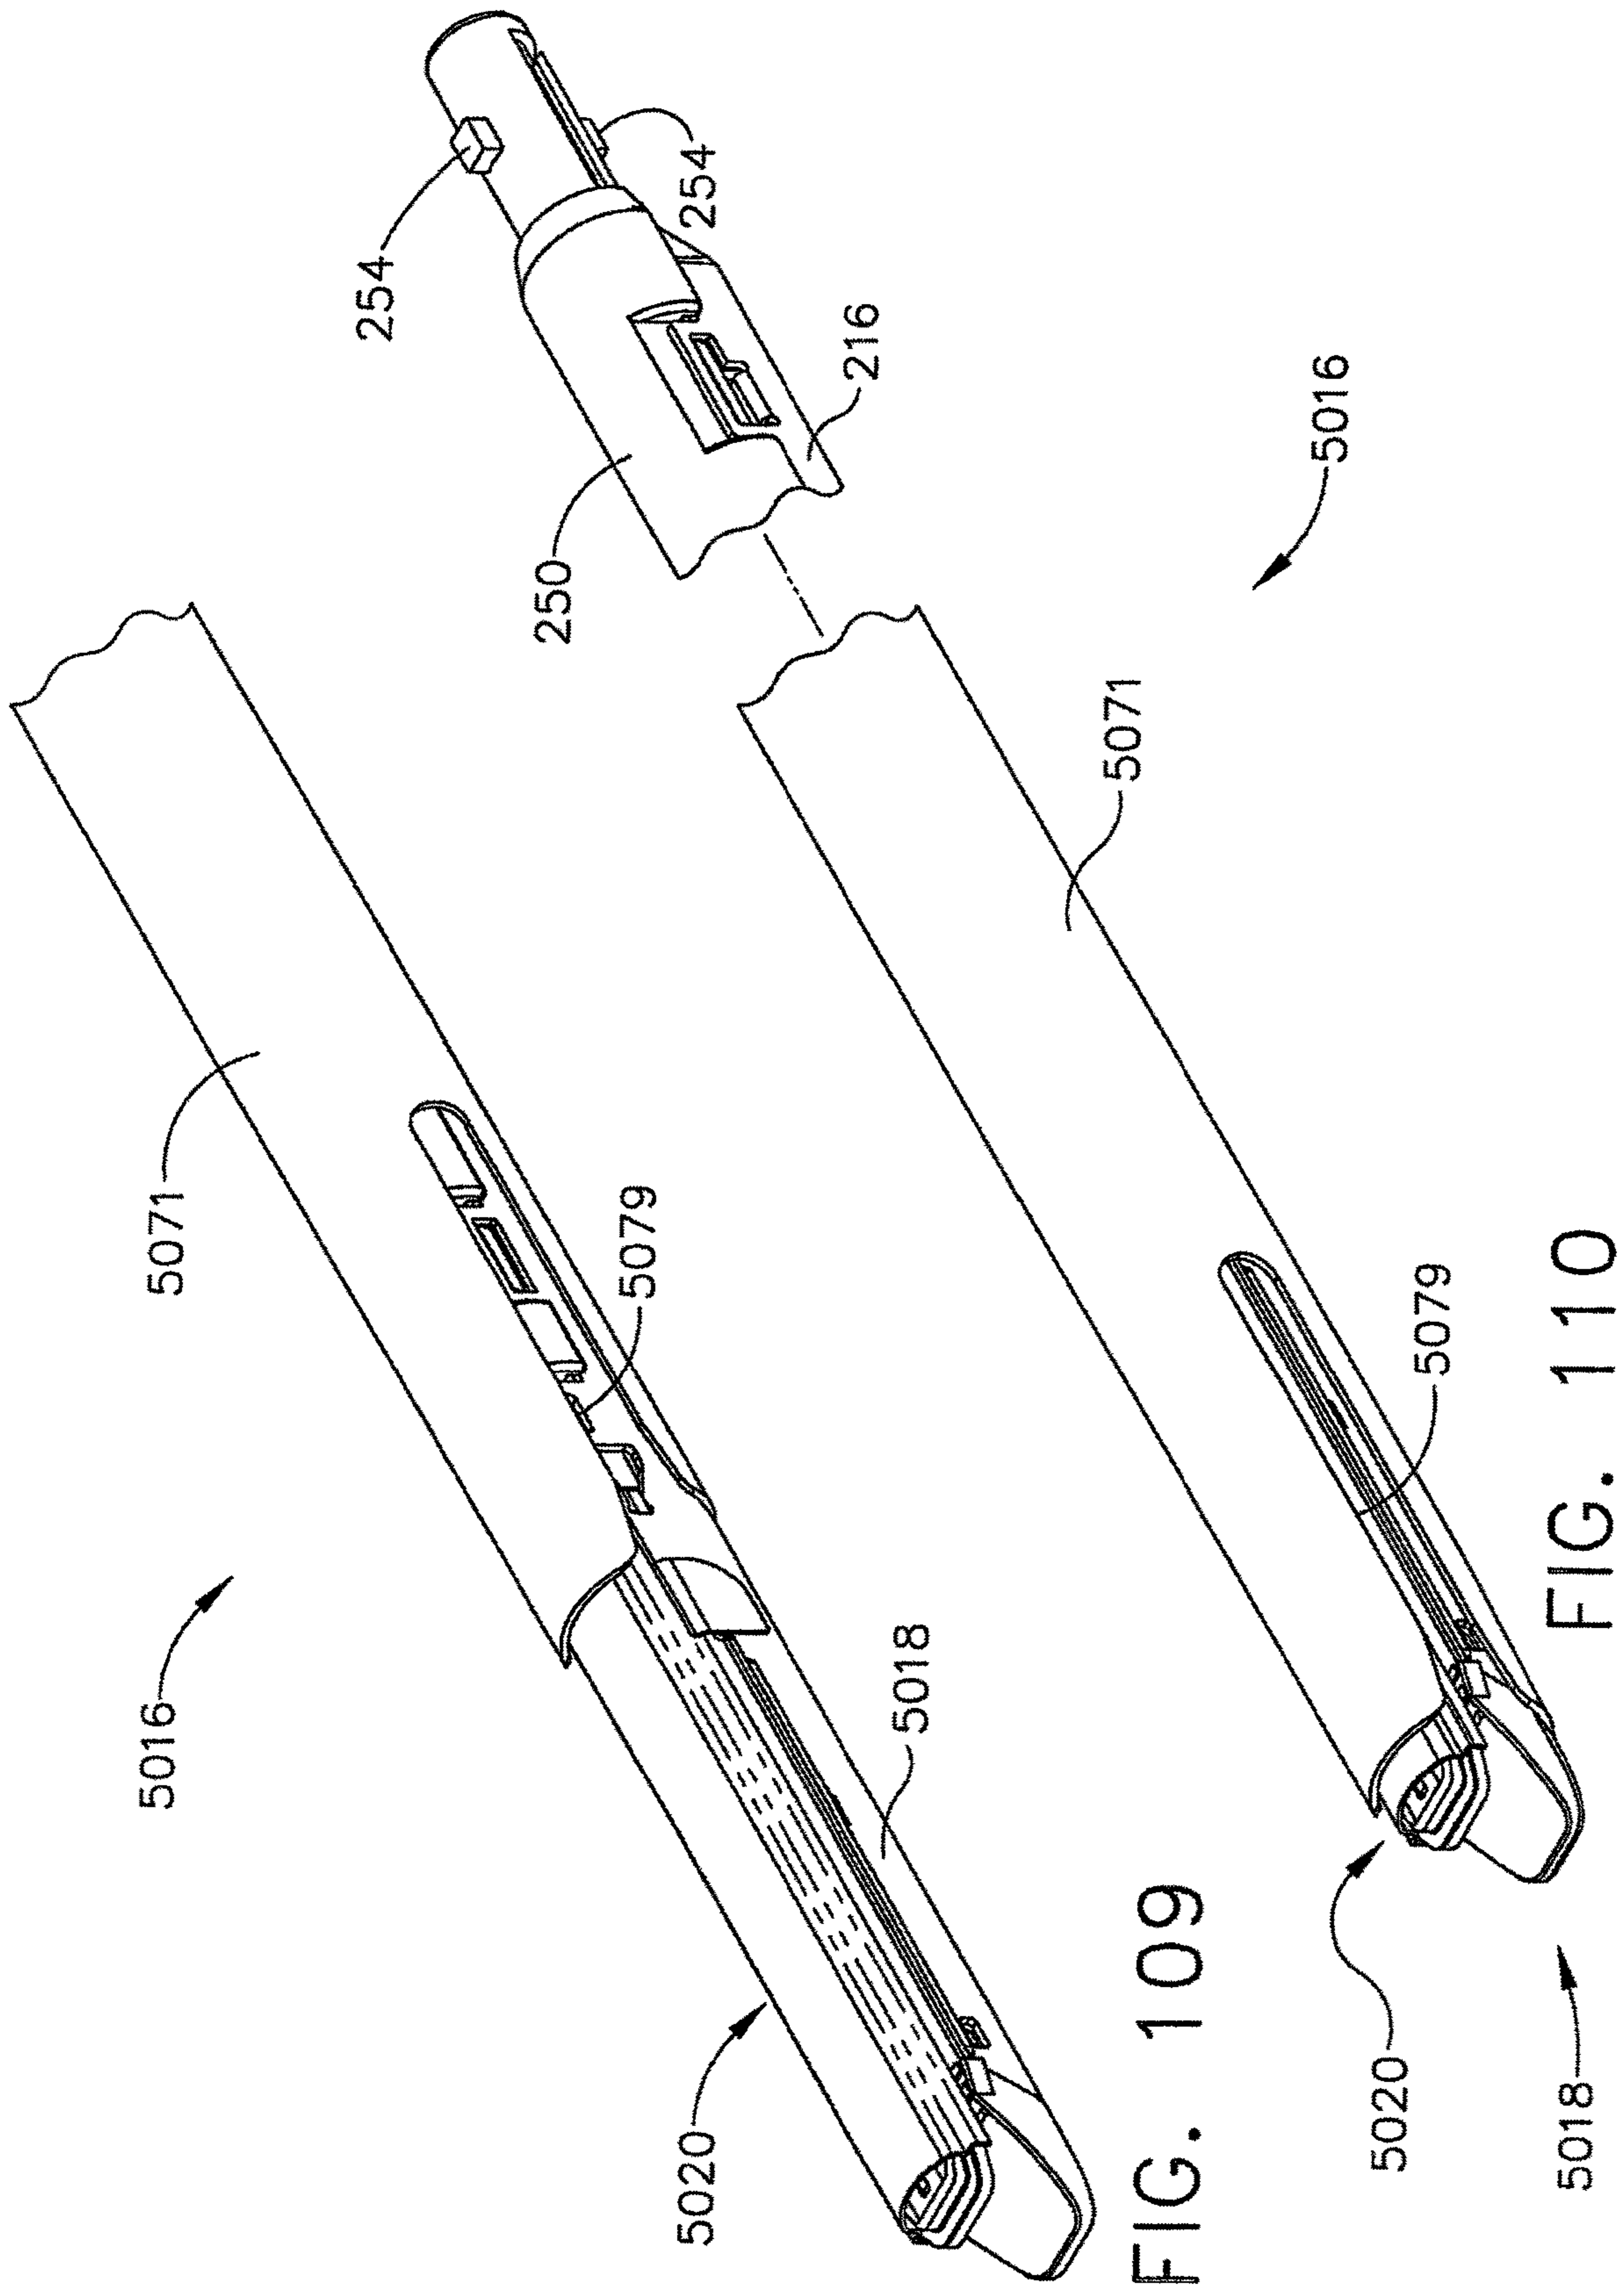


FIG. 109

FIG. 110

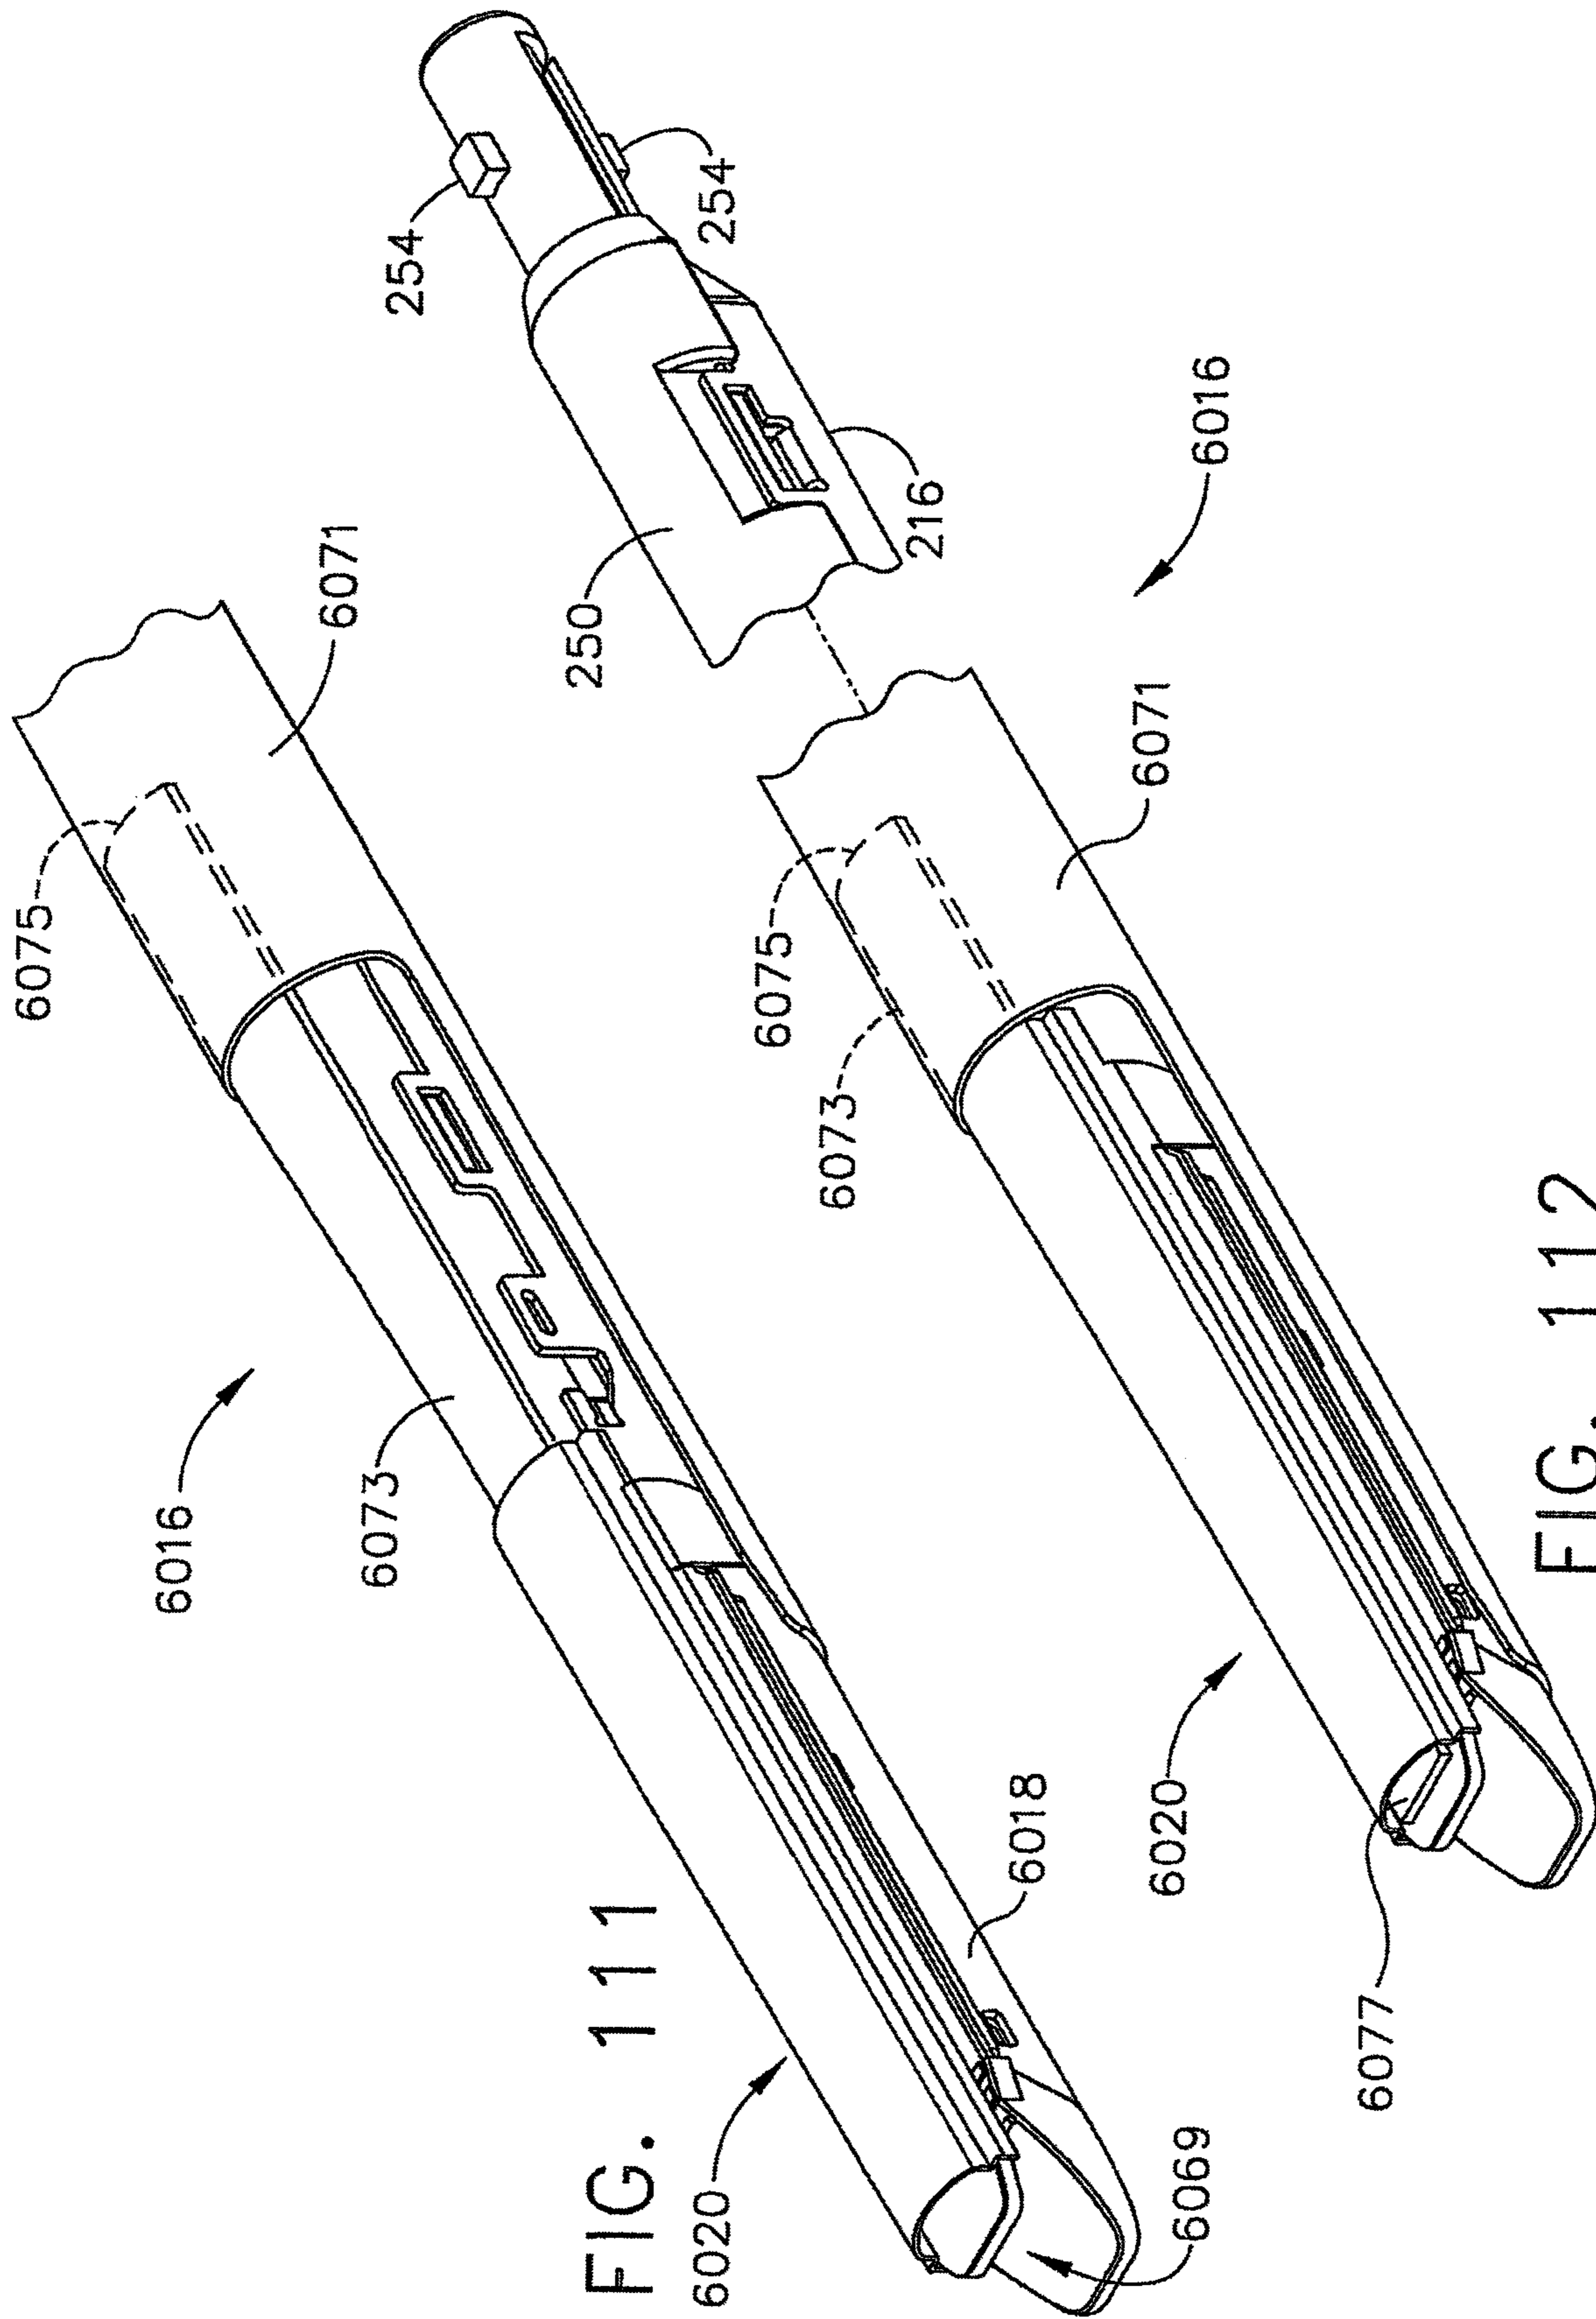


FIG. 111

FIG. 112

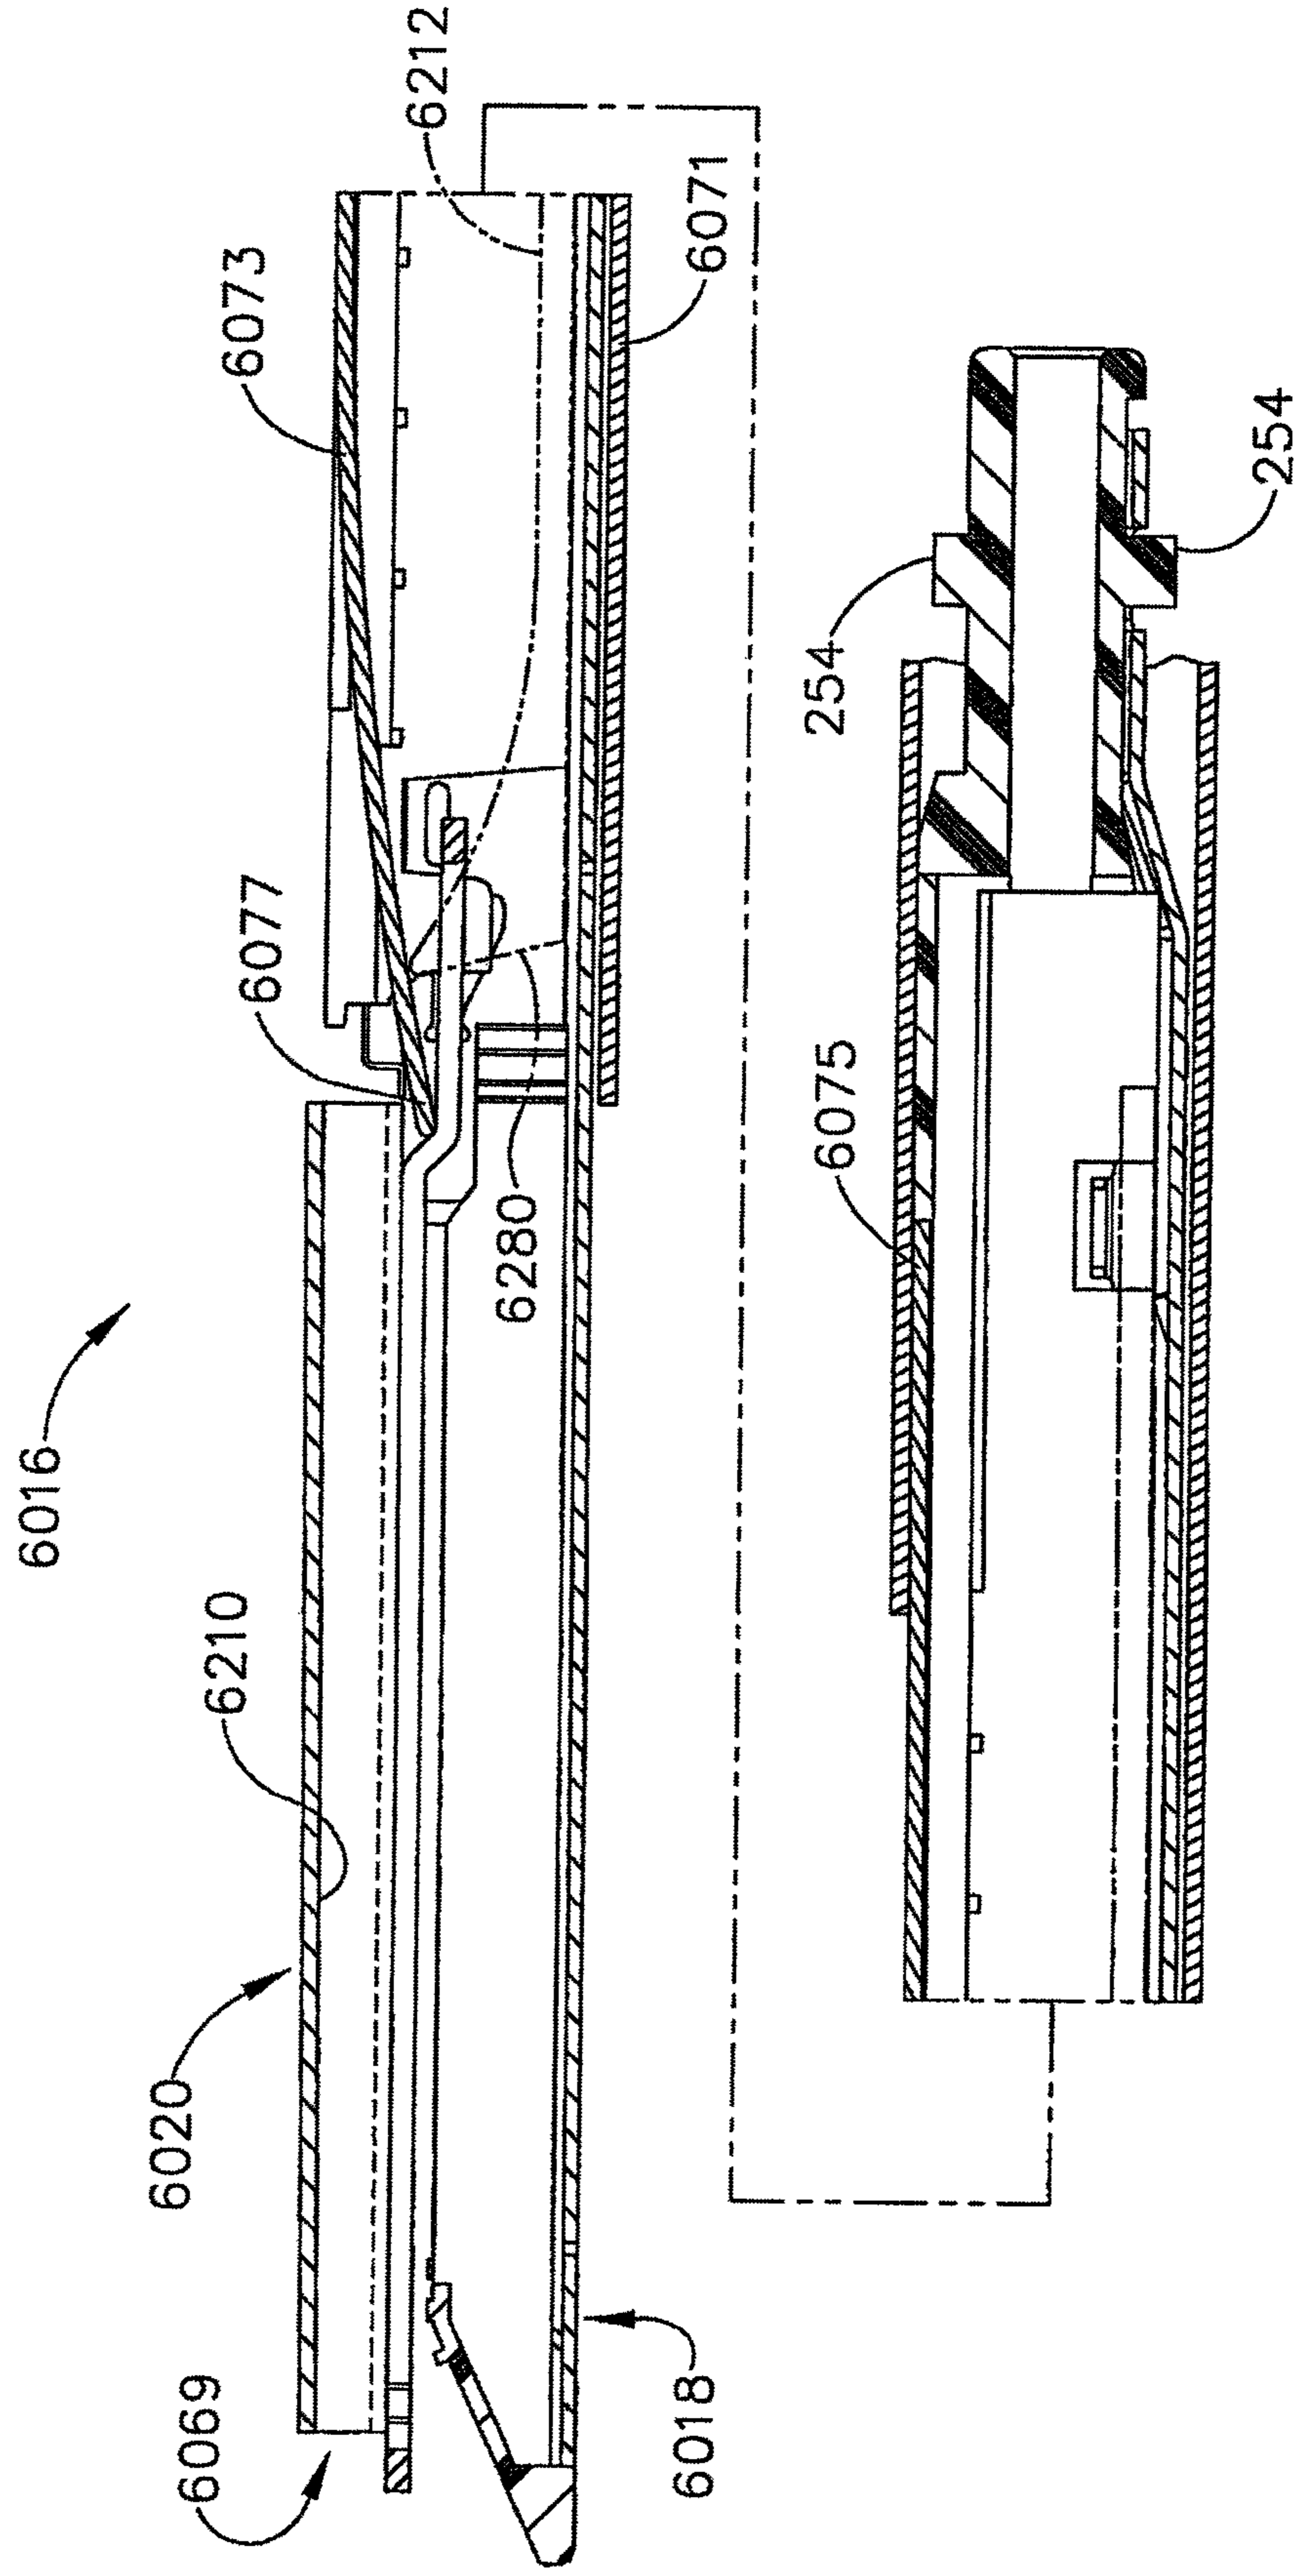


FIG. 113



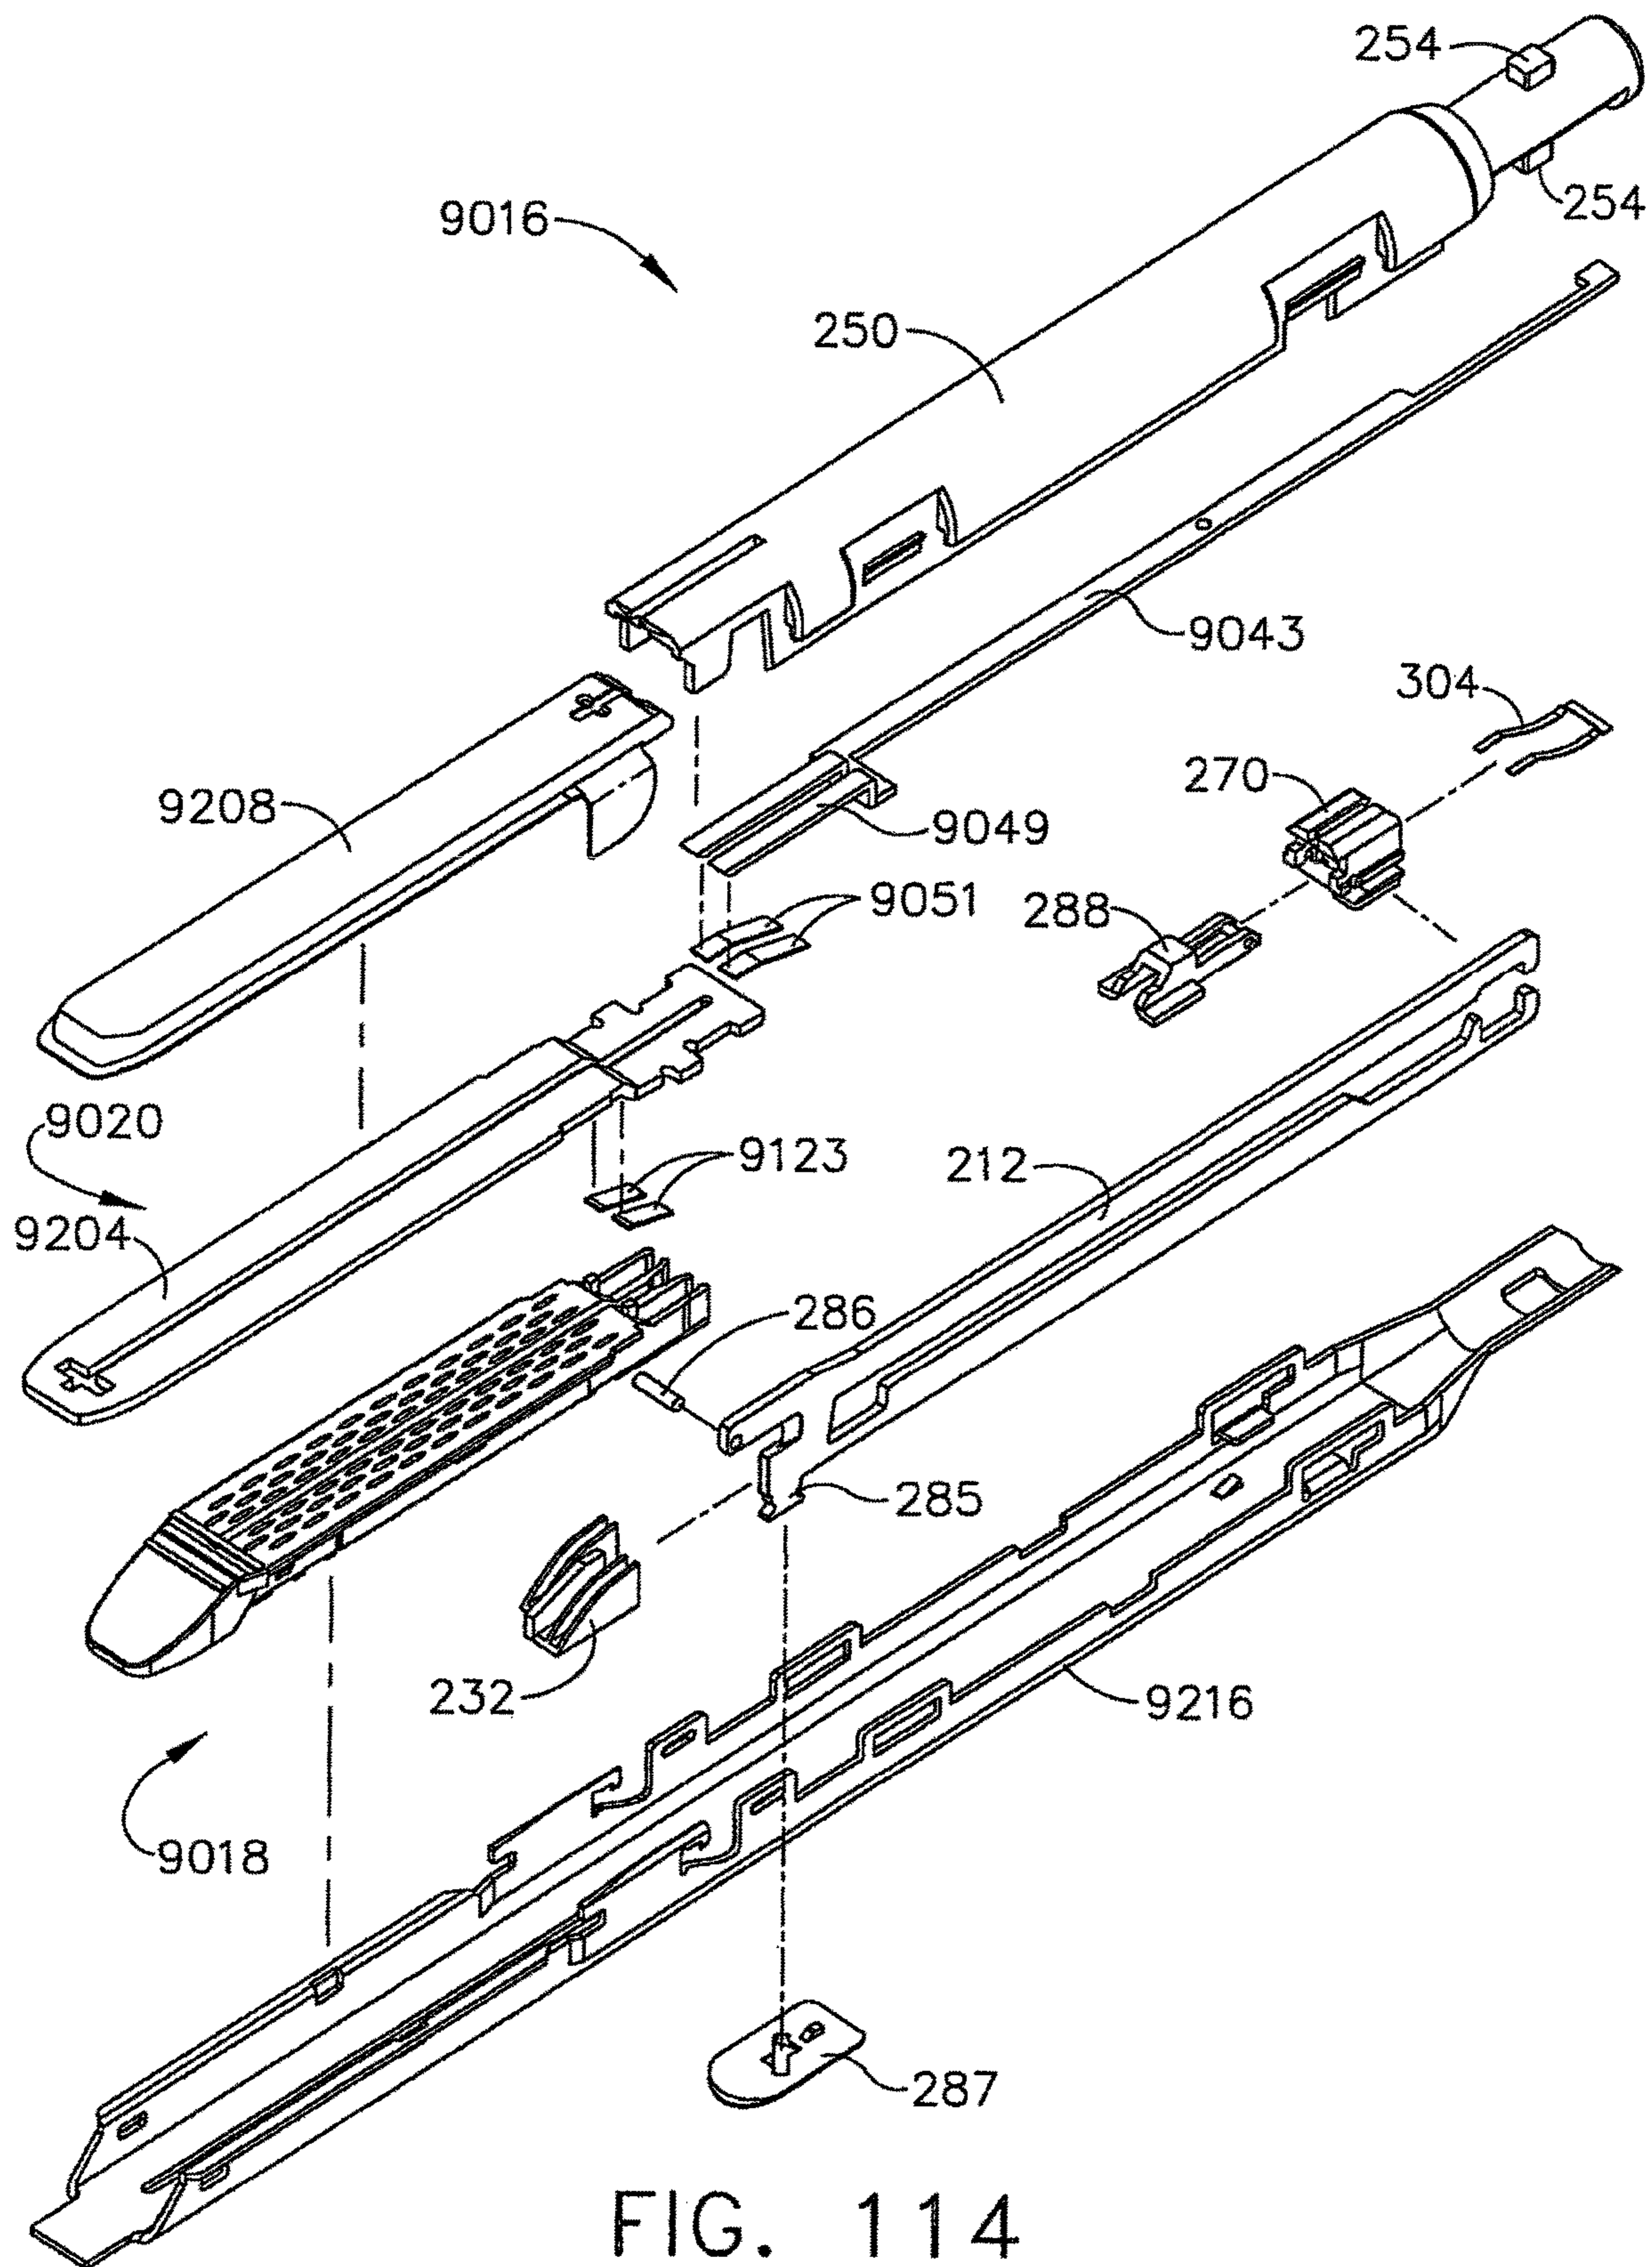


FIG. 114

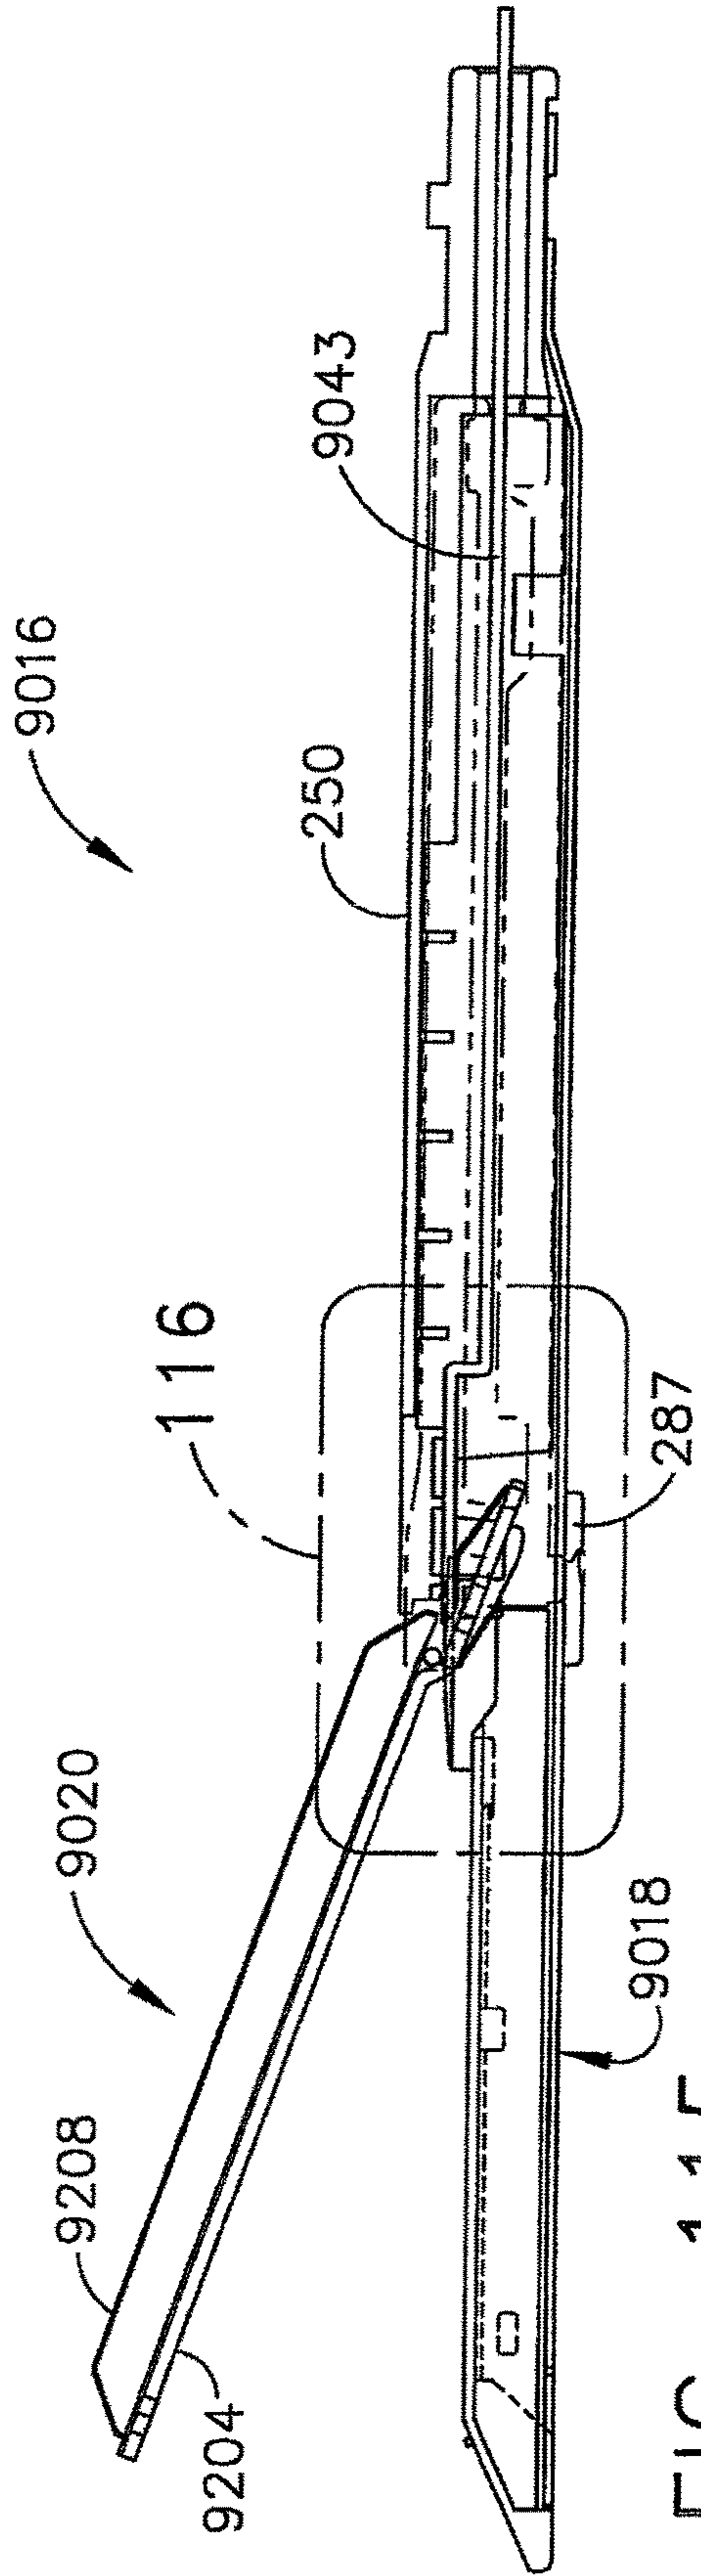


FIG. 115

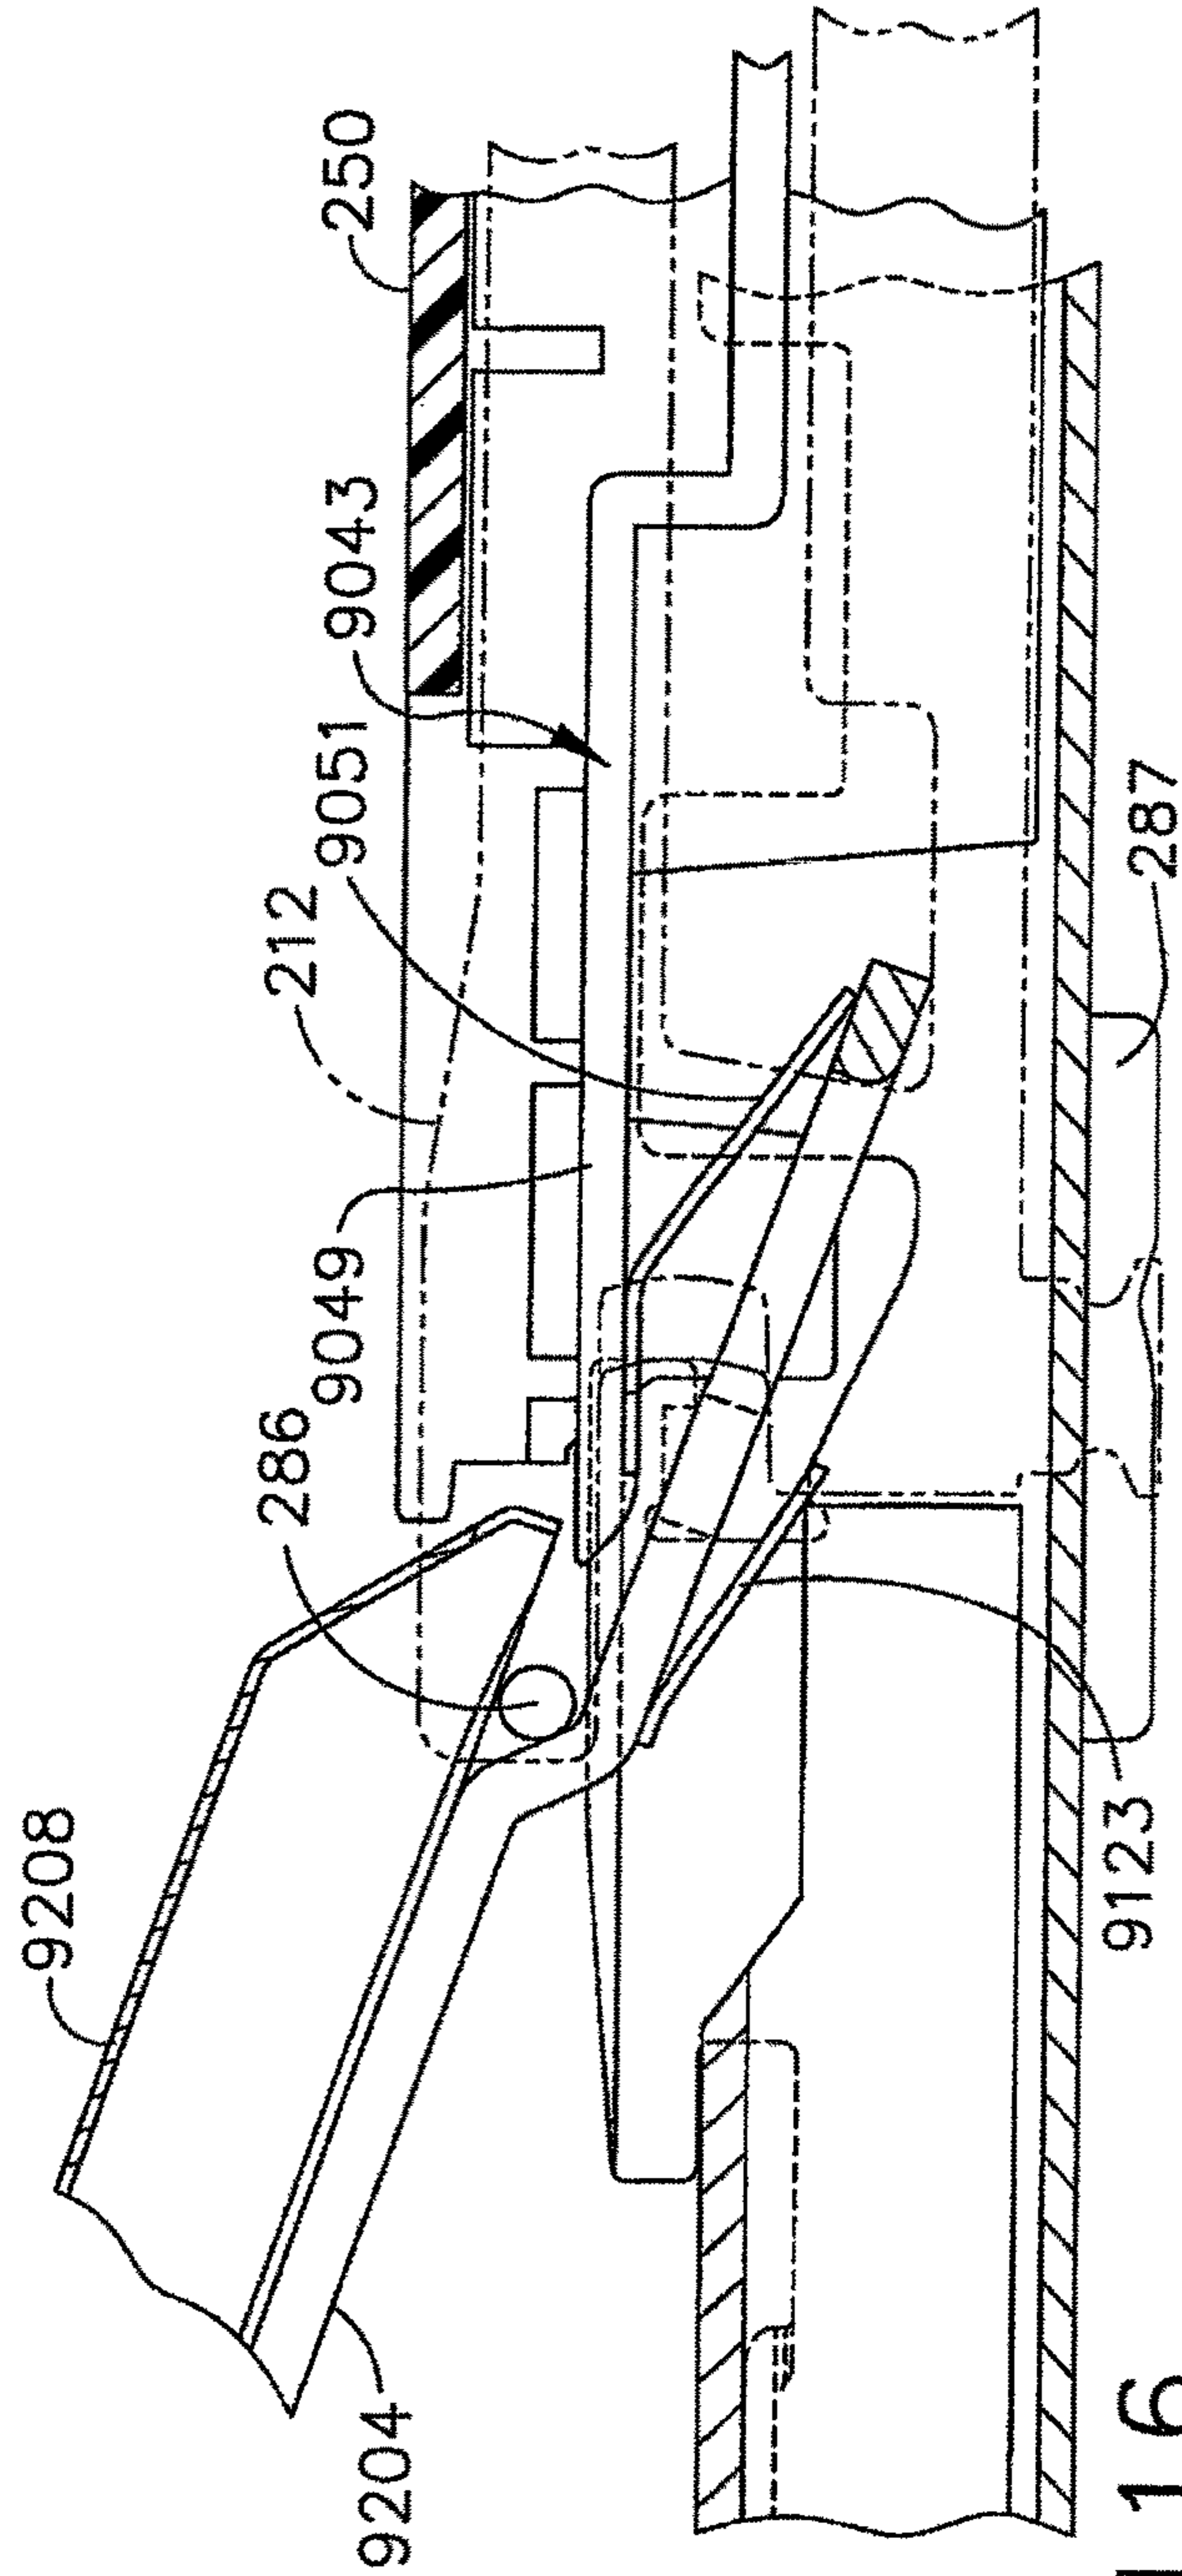


FIG. 116

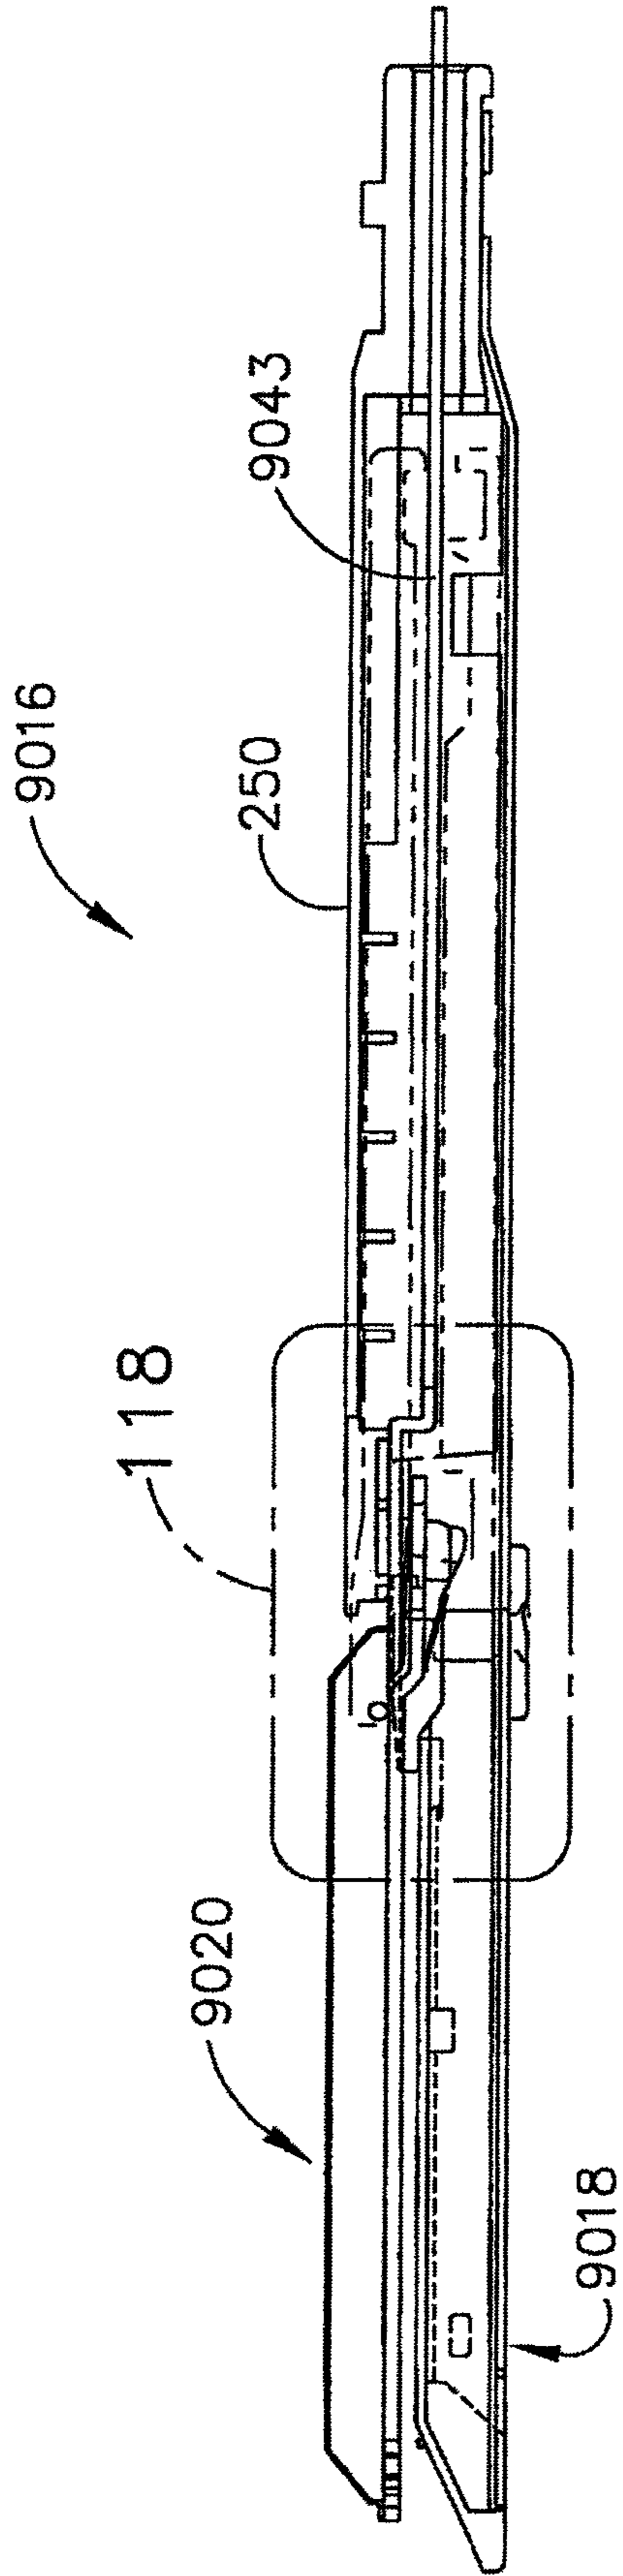


FIG. 1117

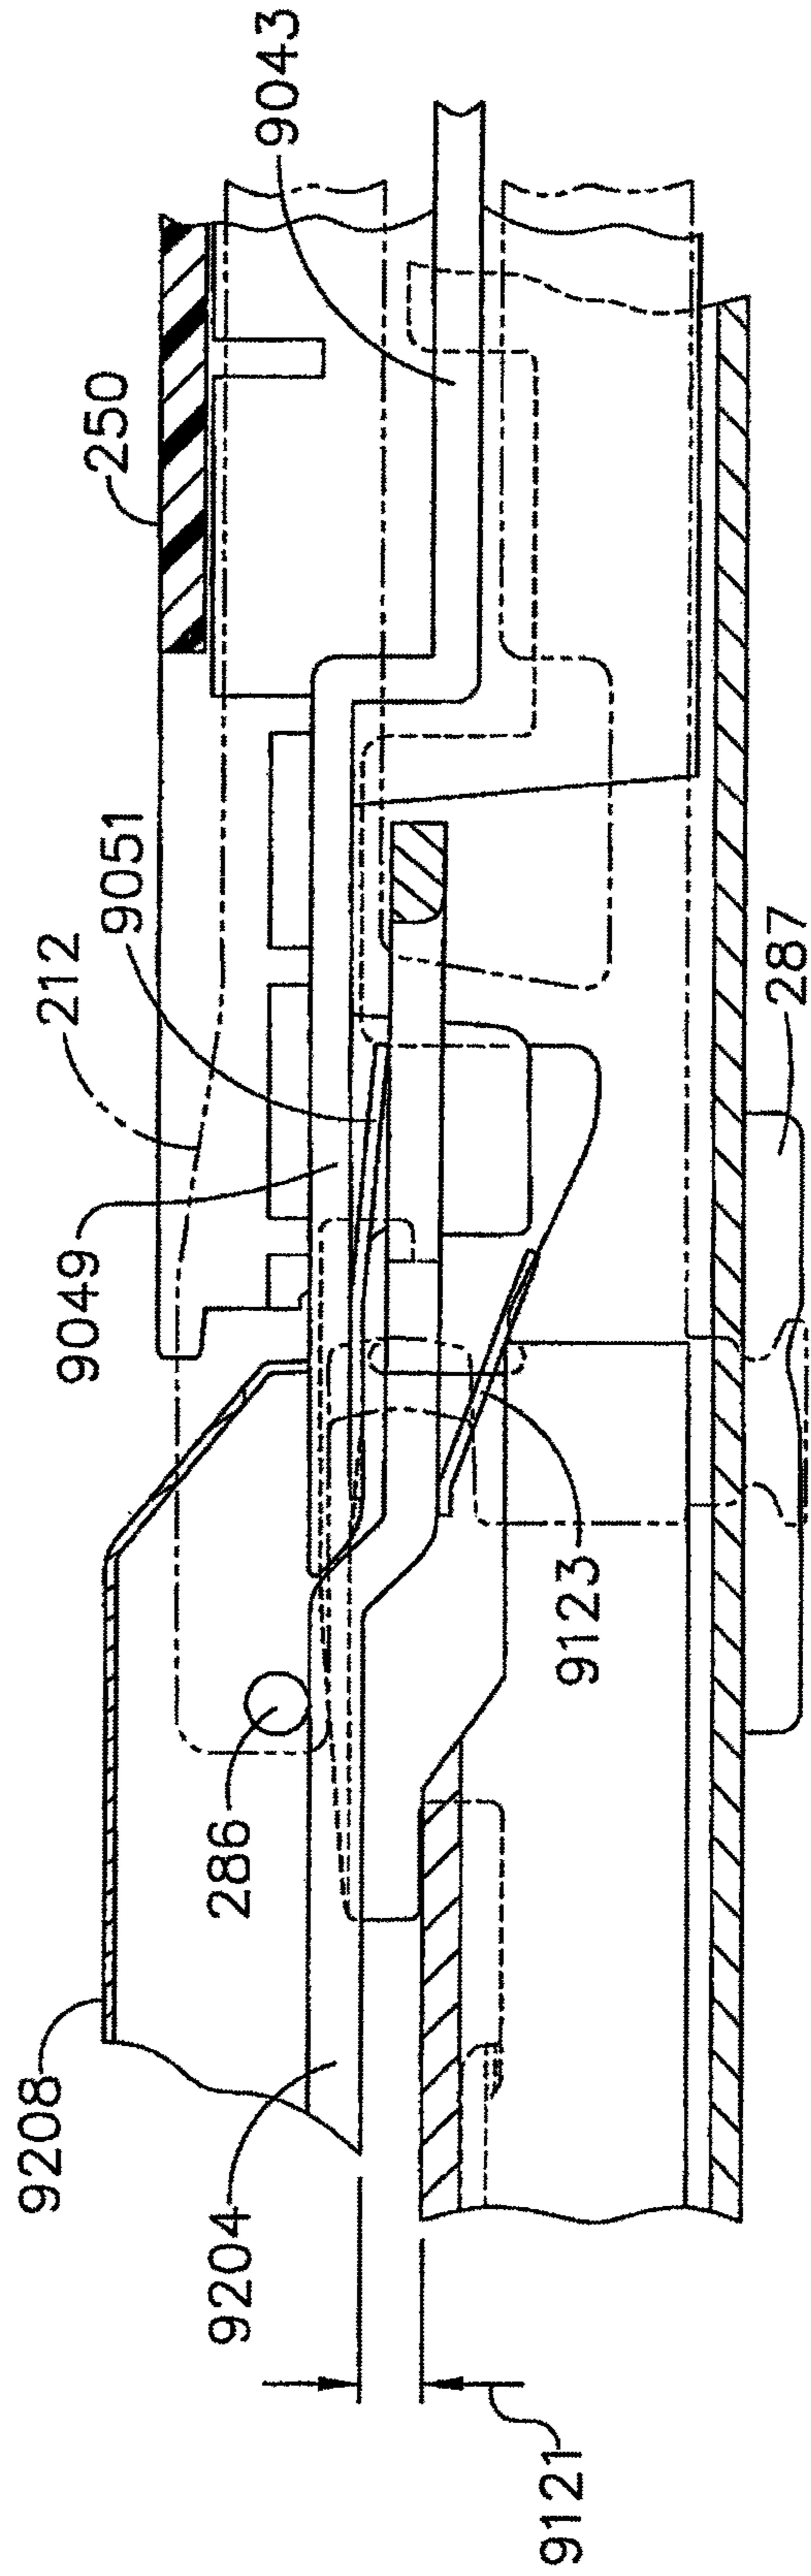


FIG. 1118

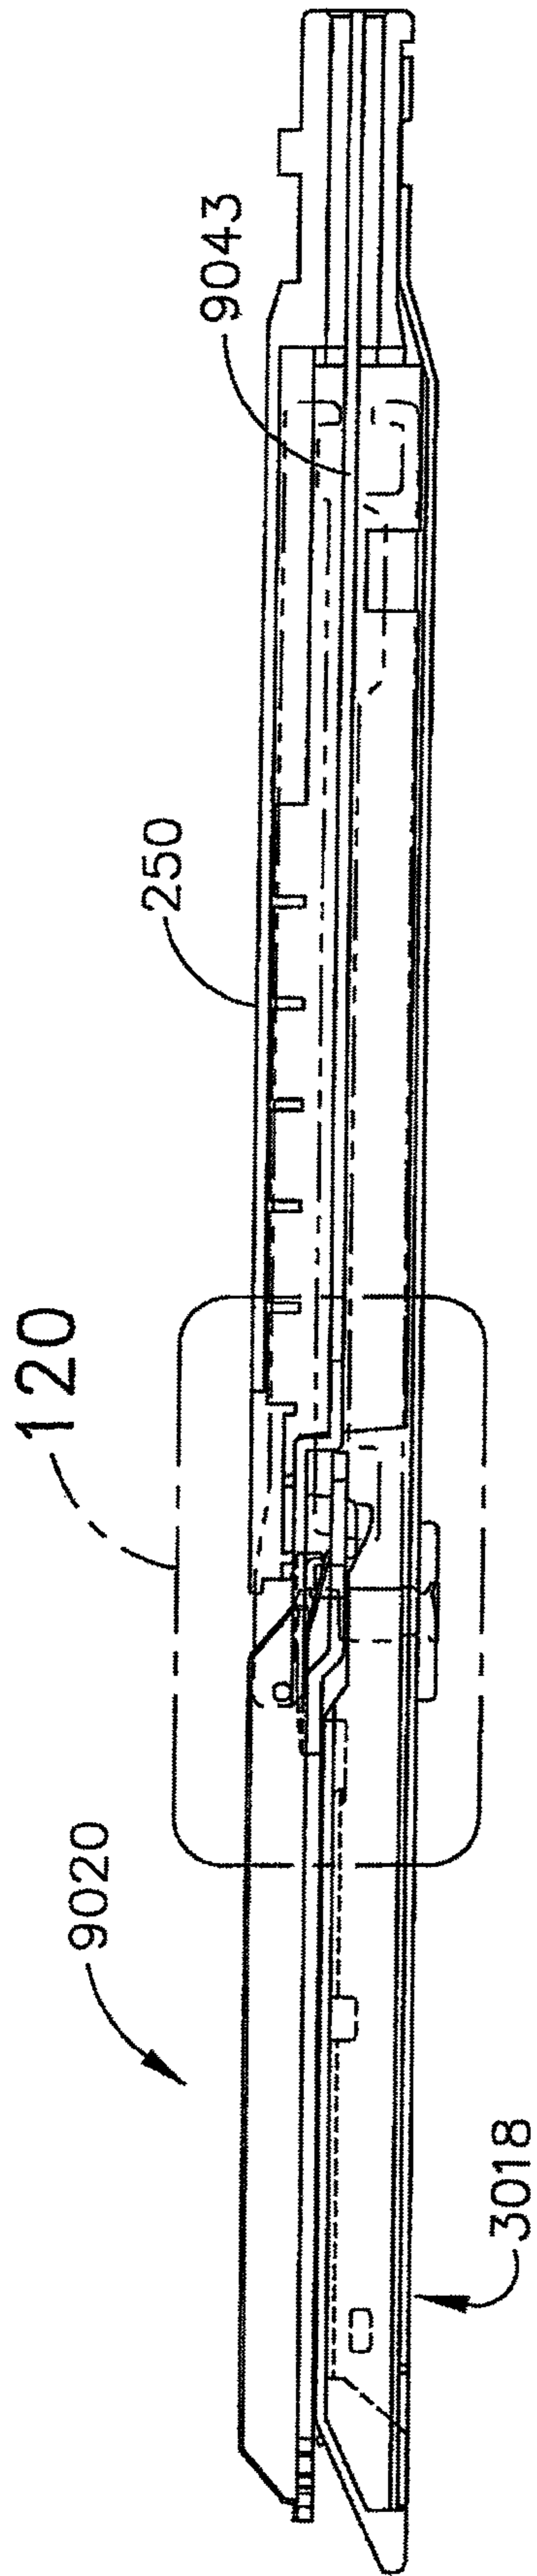


FIG. 119

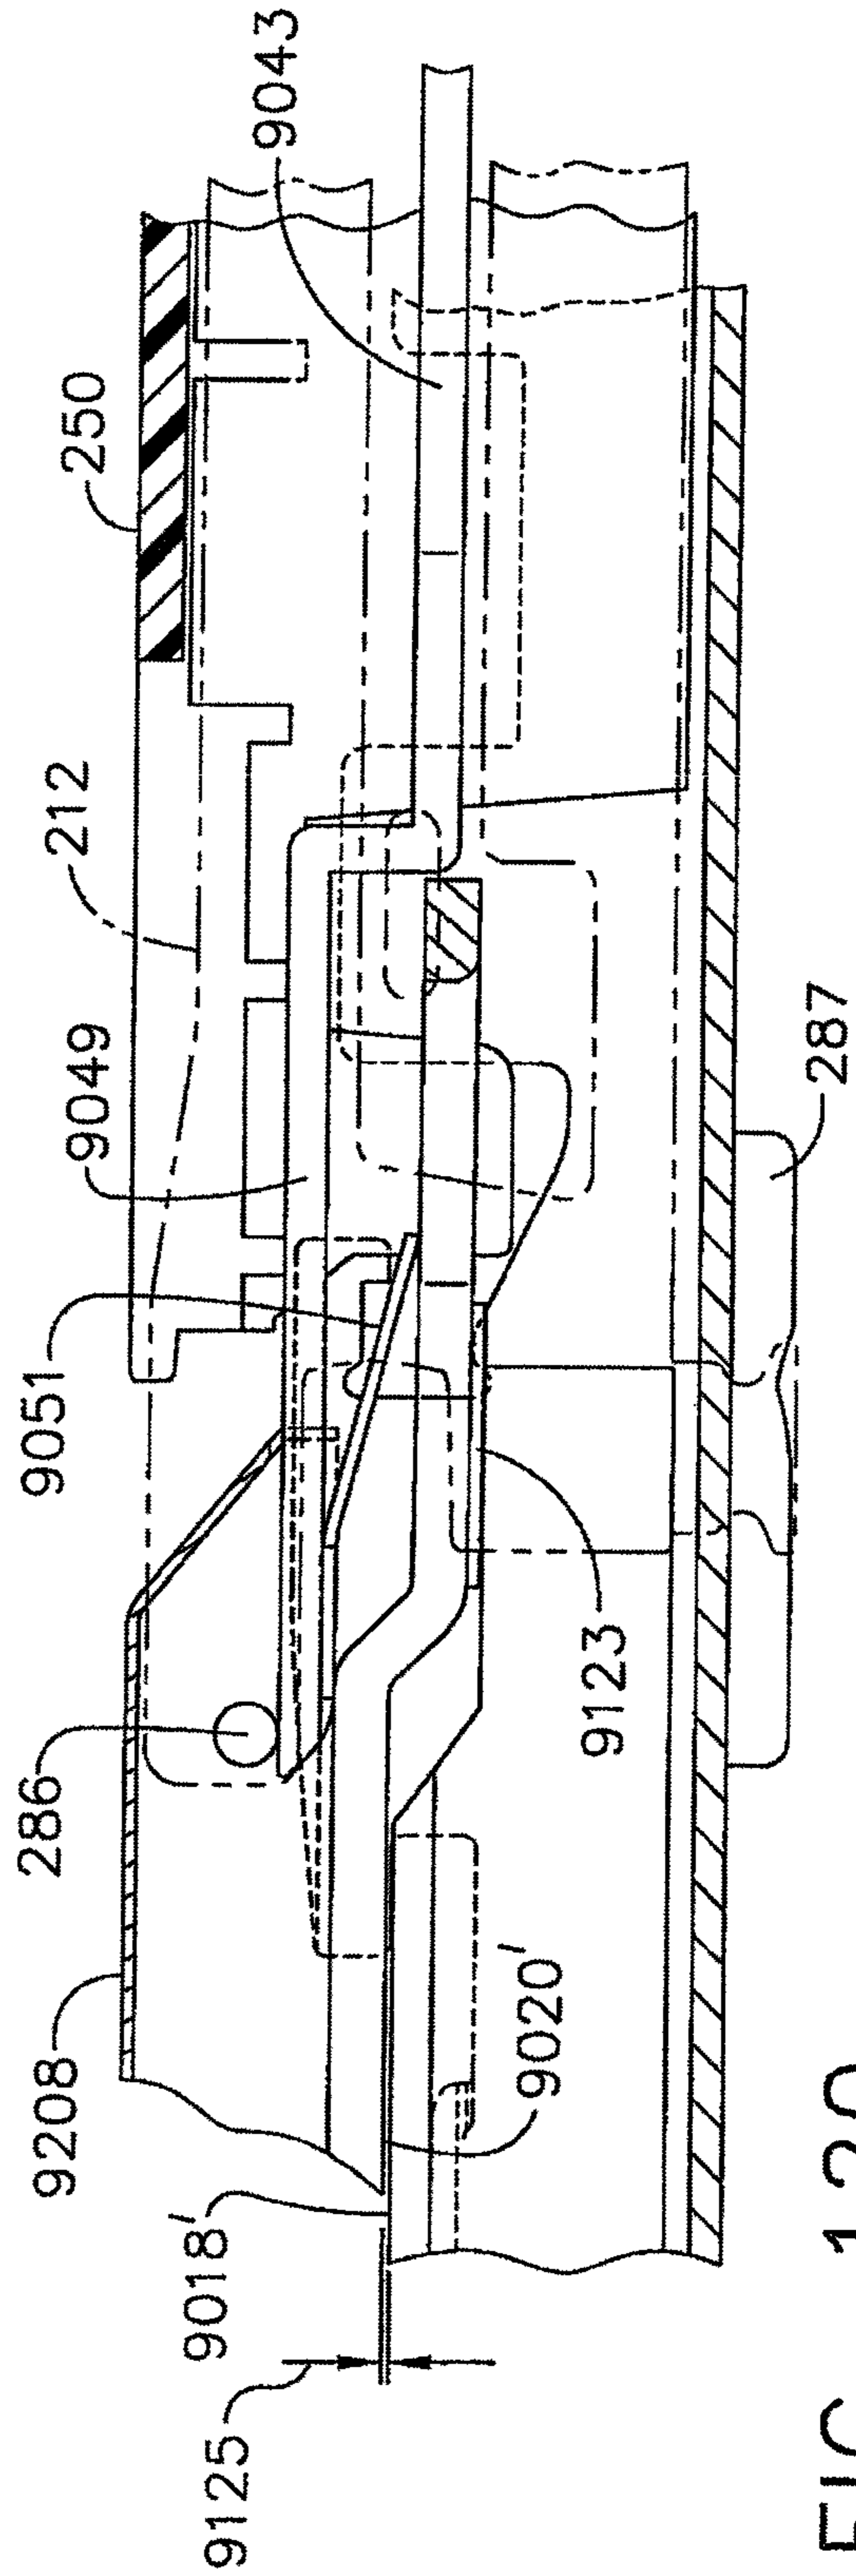


FIG. 120

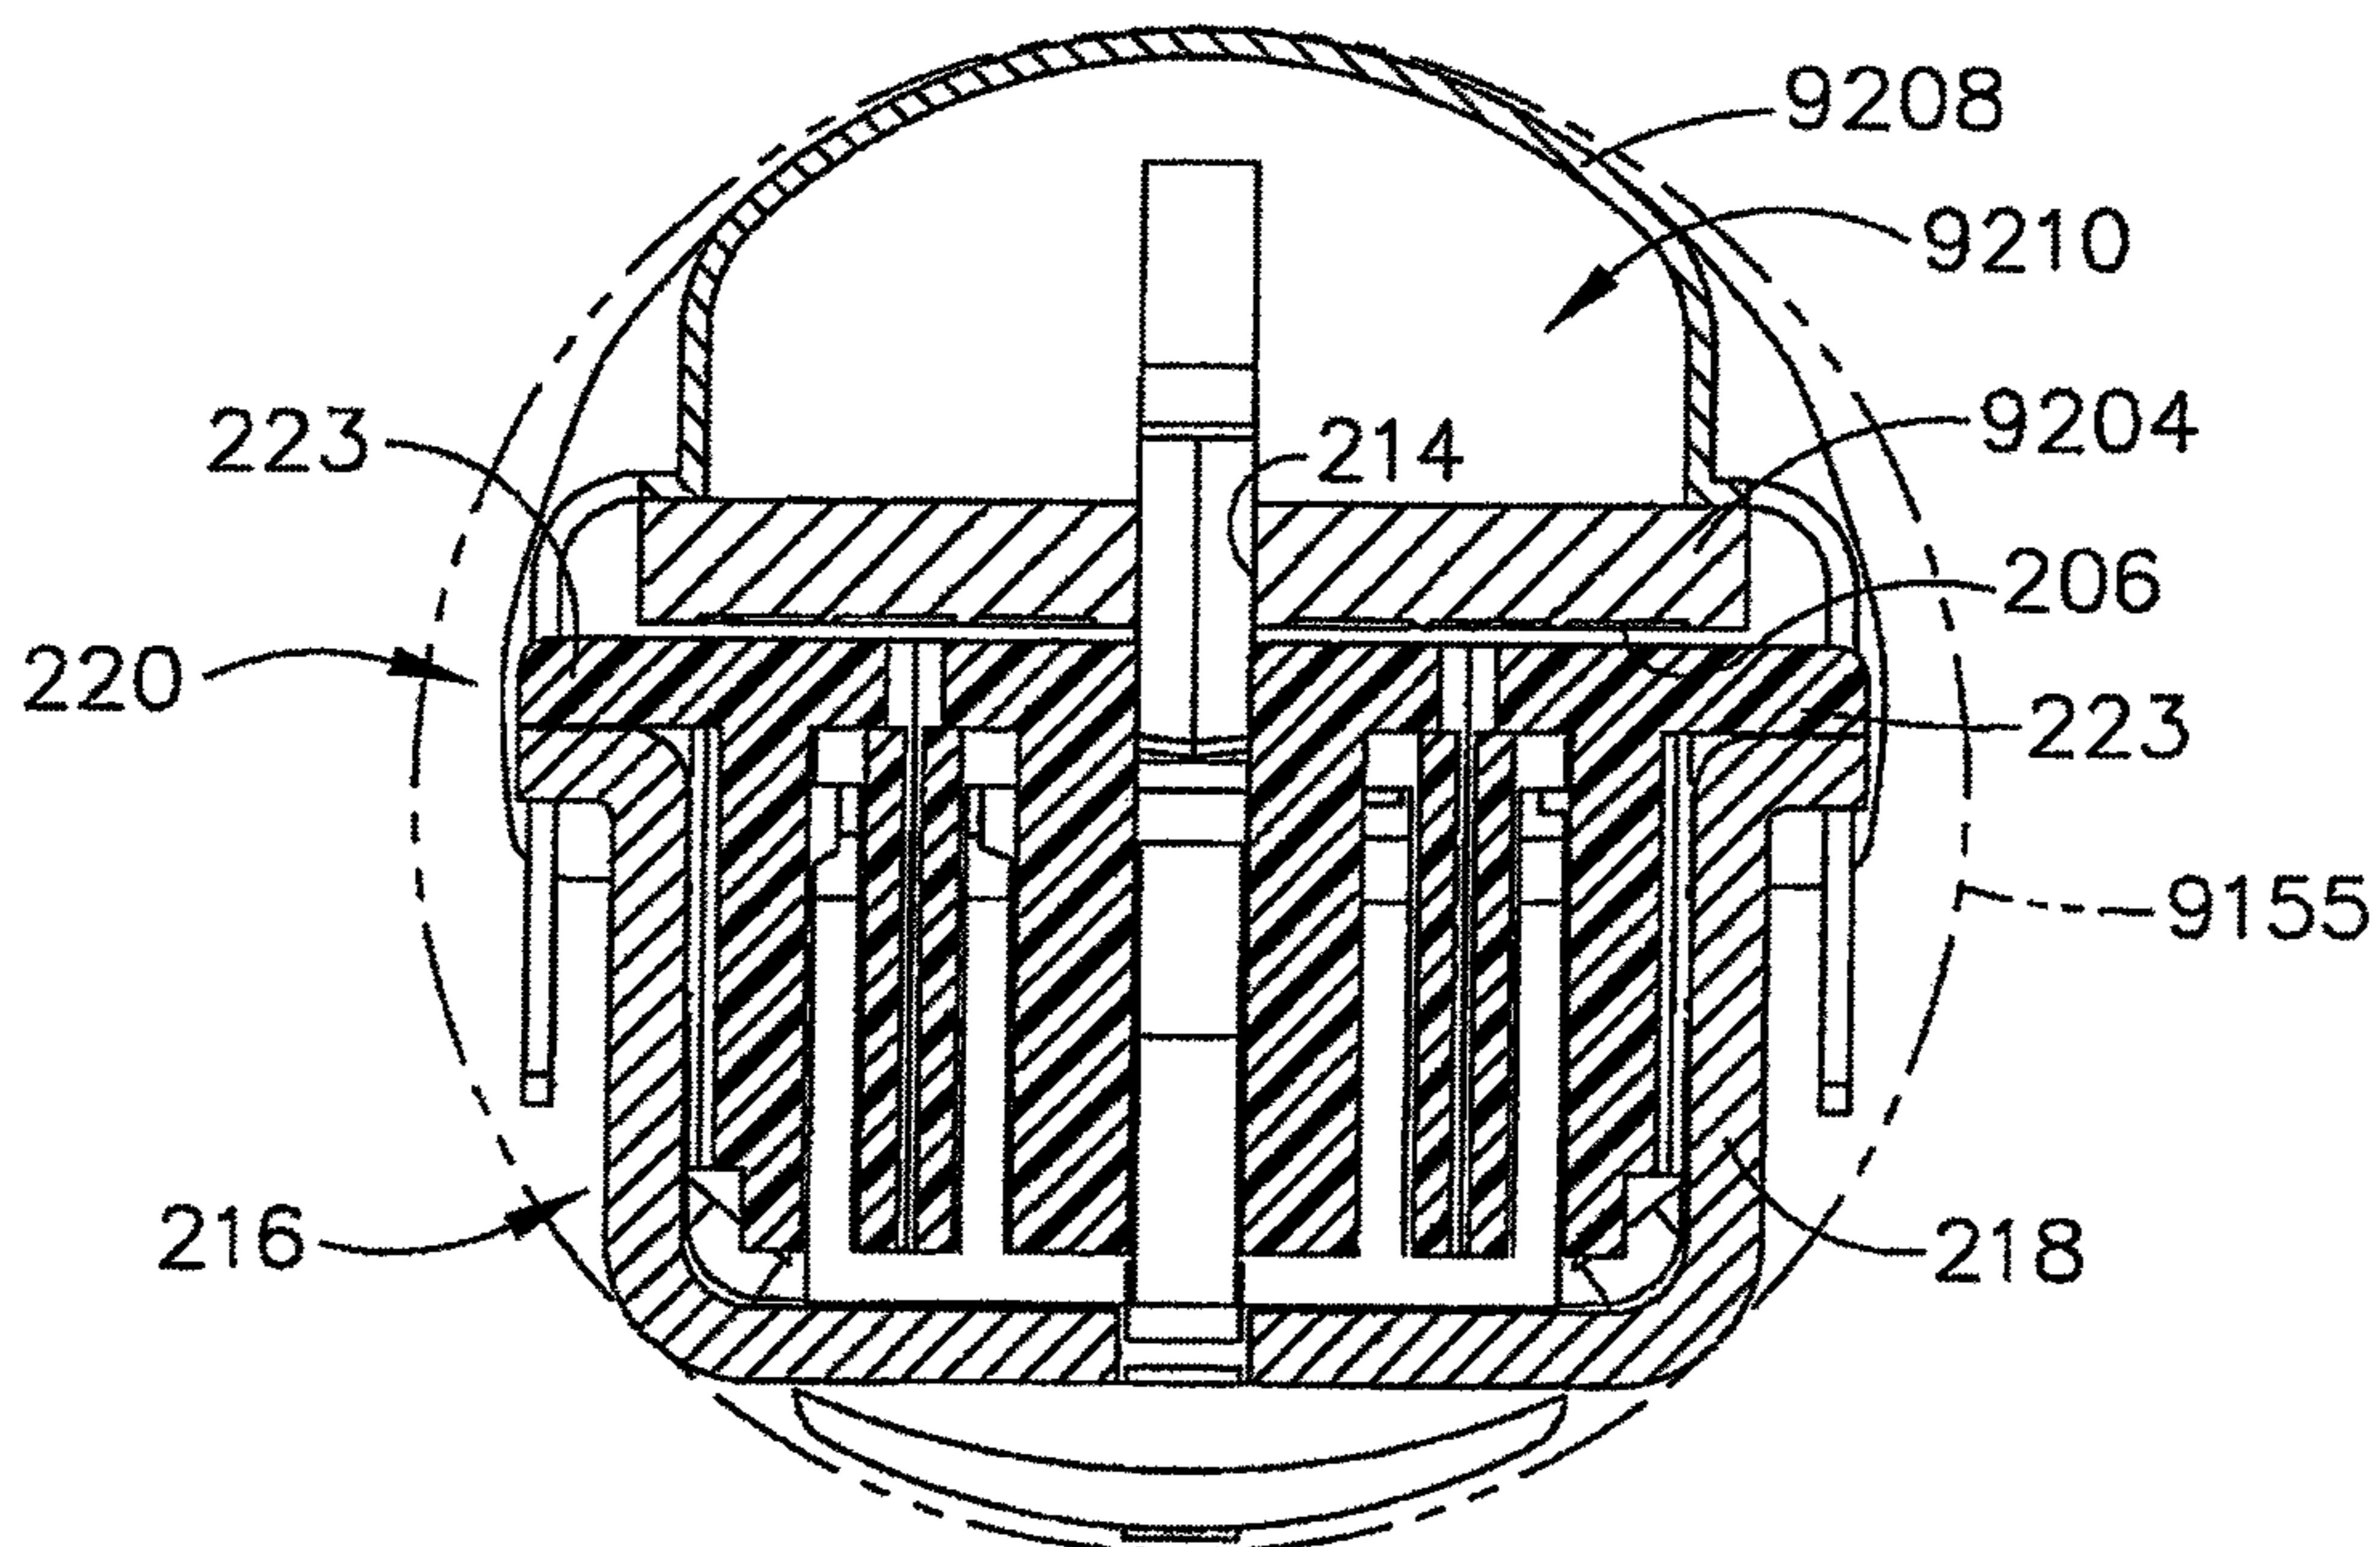


FIG. 121

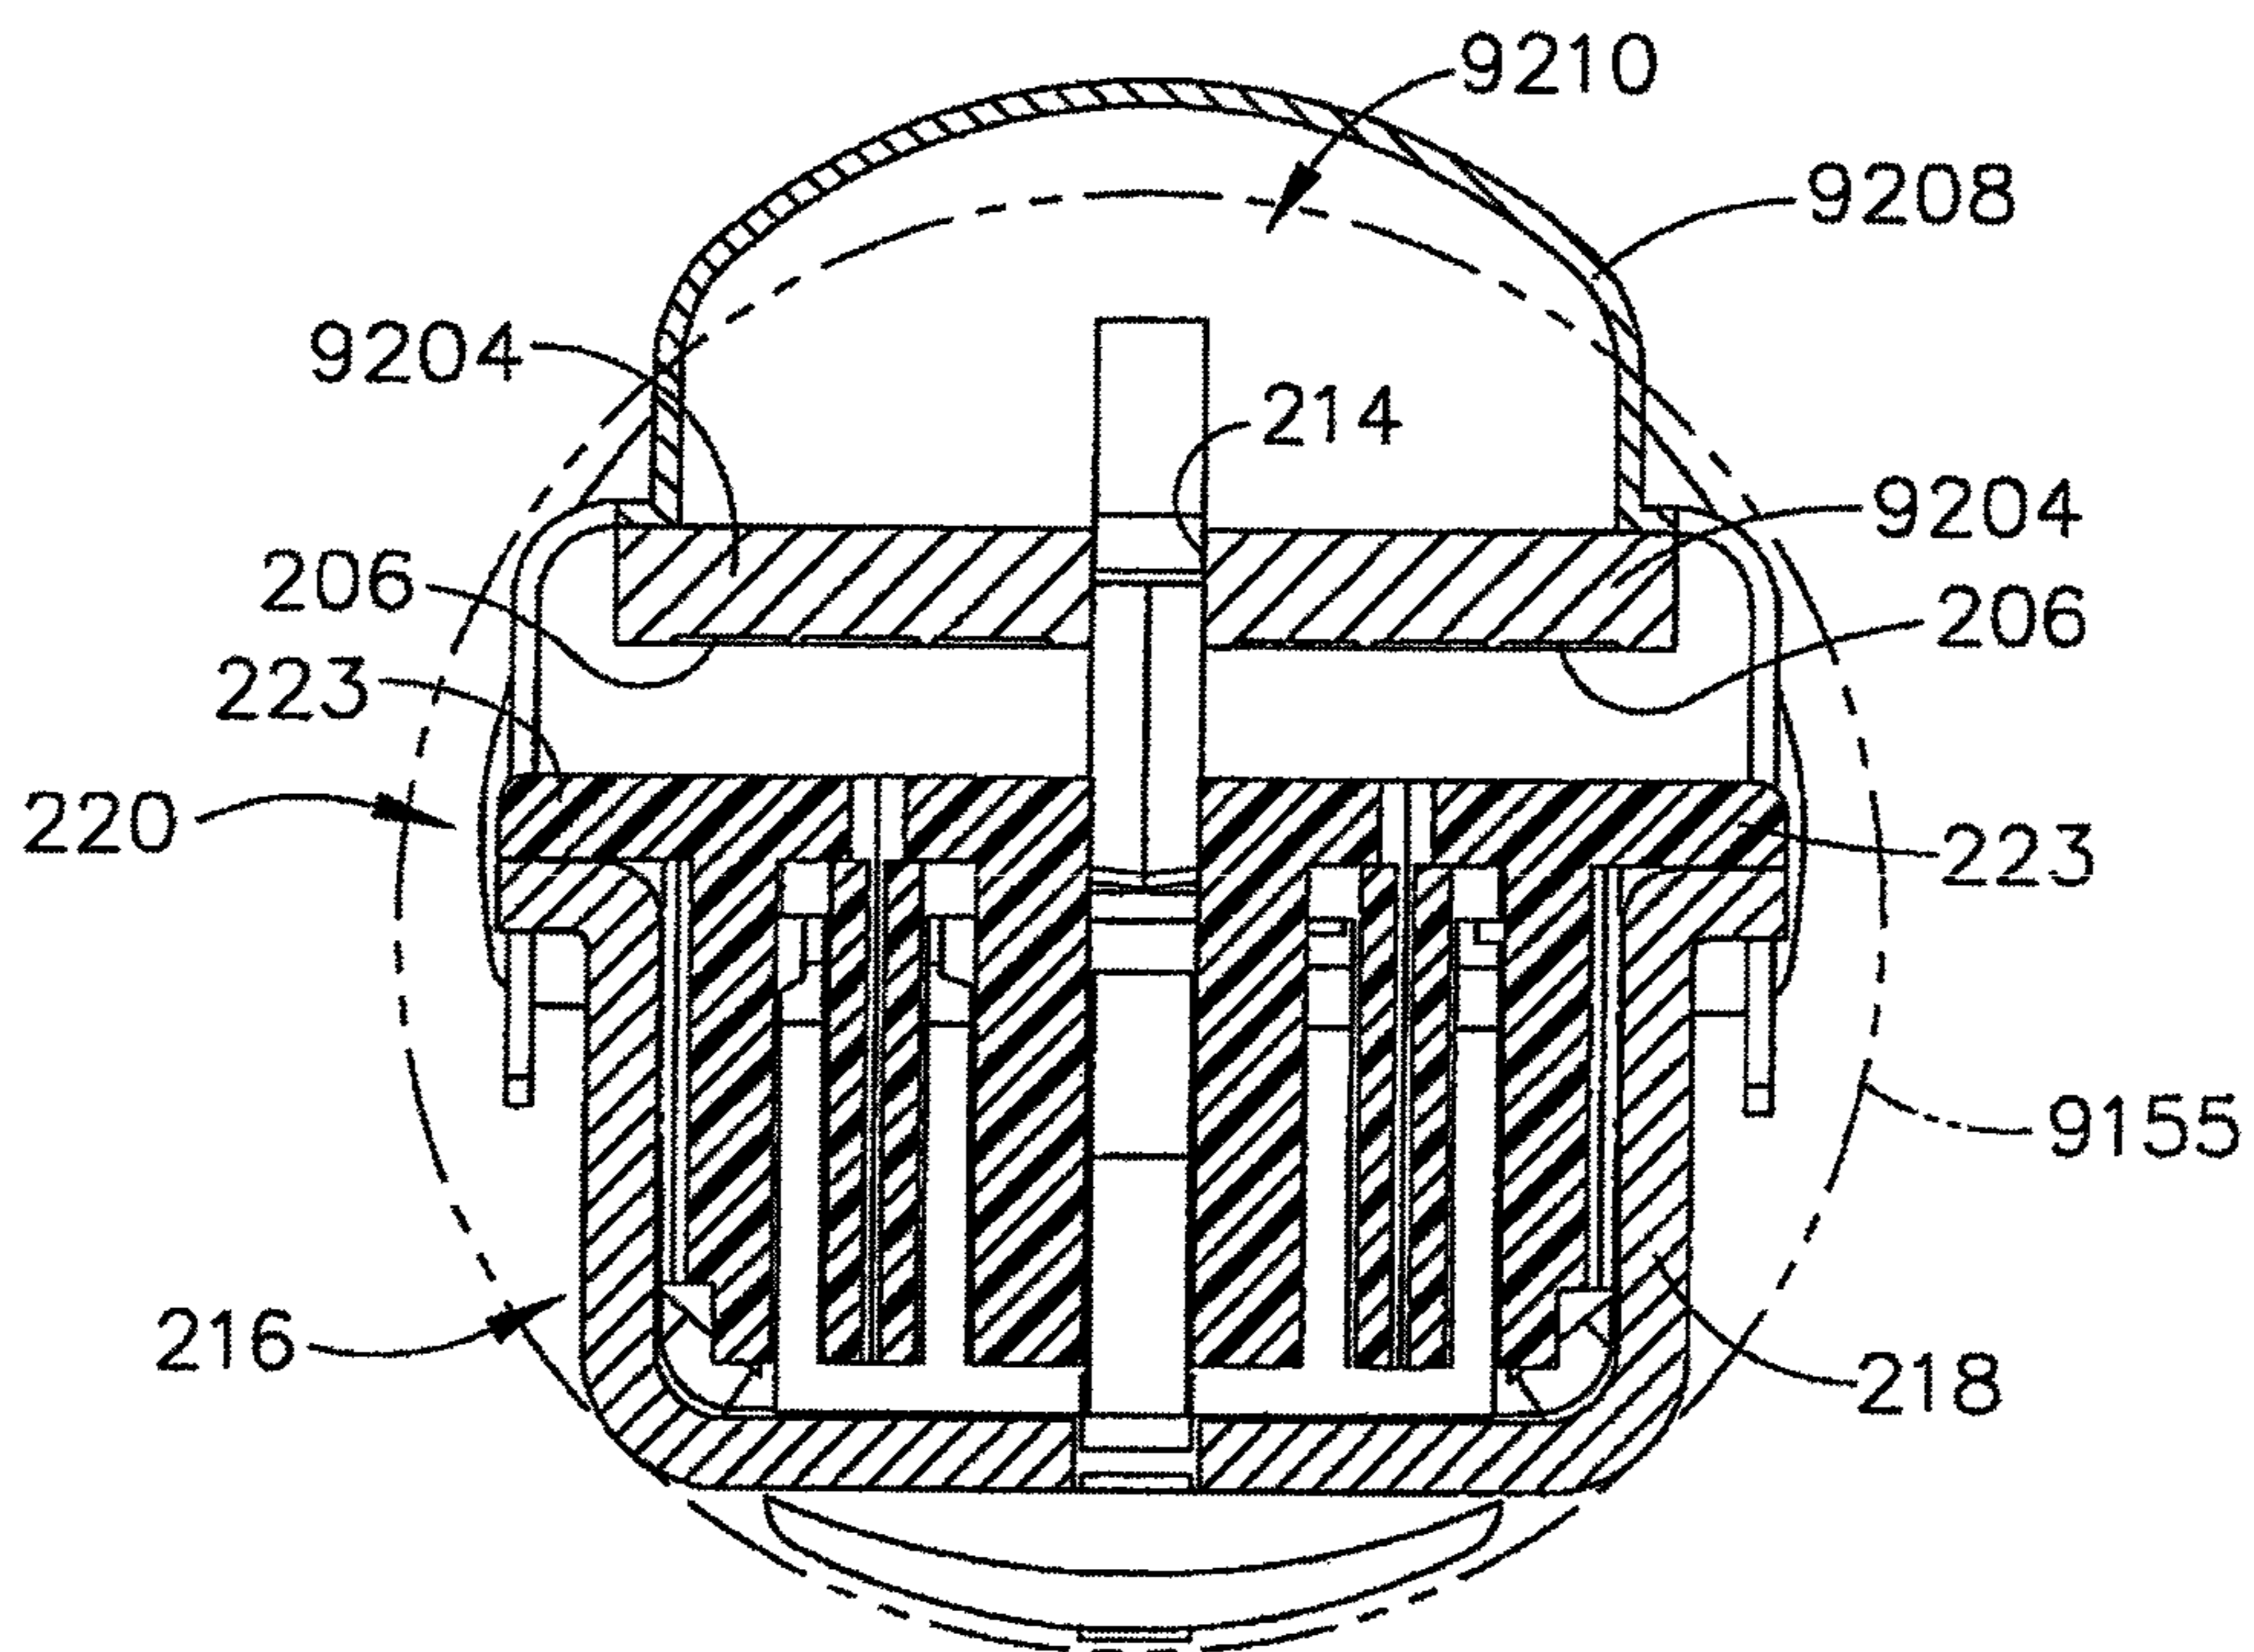


FIG. 122

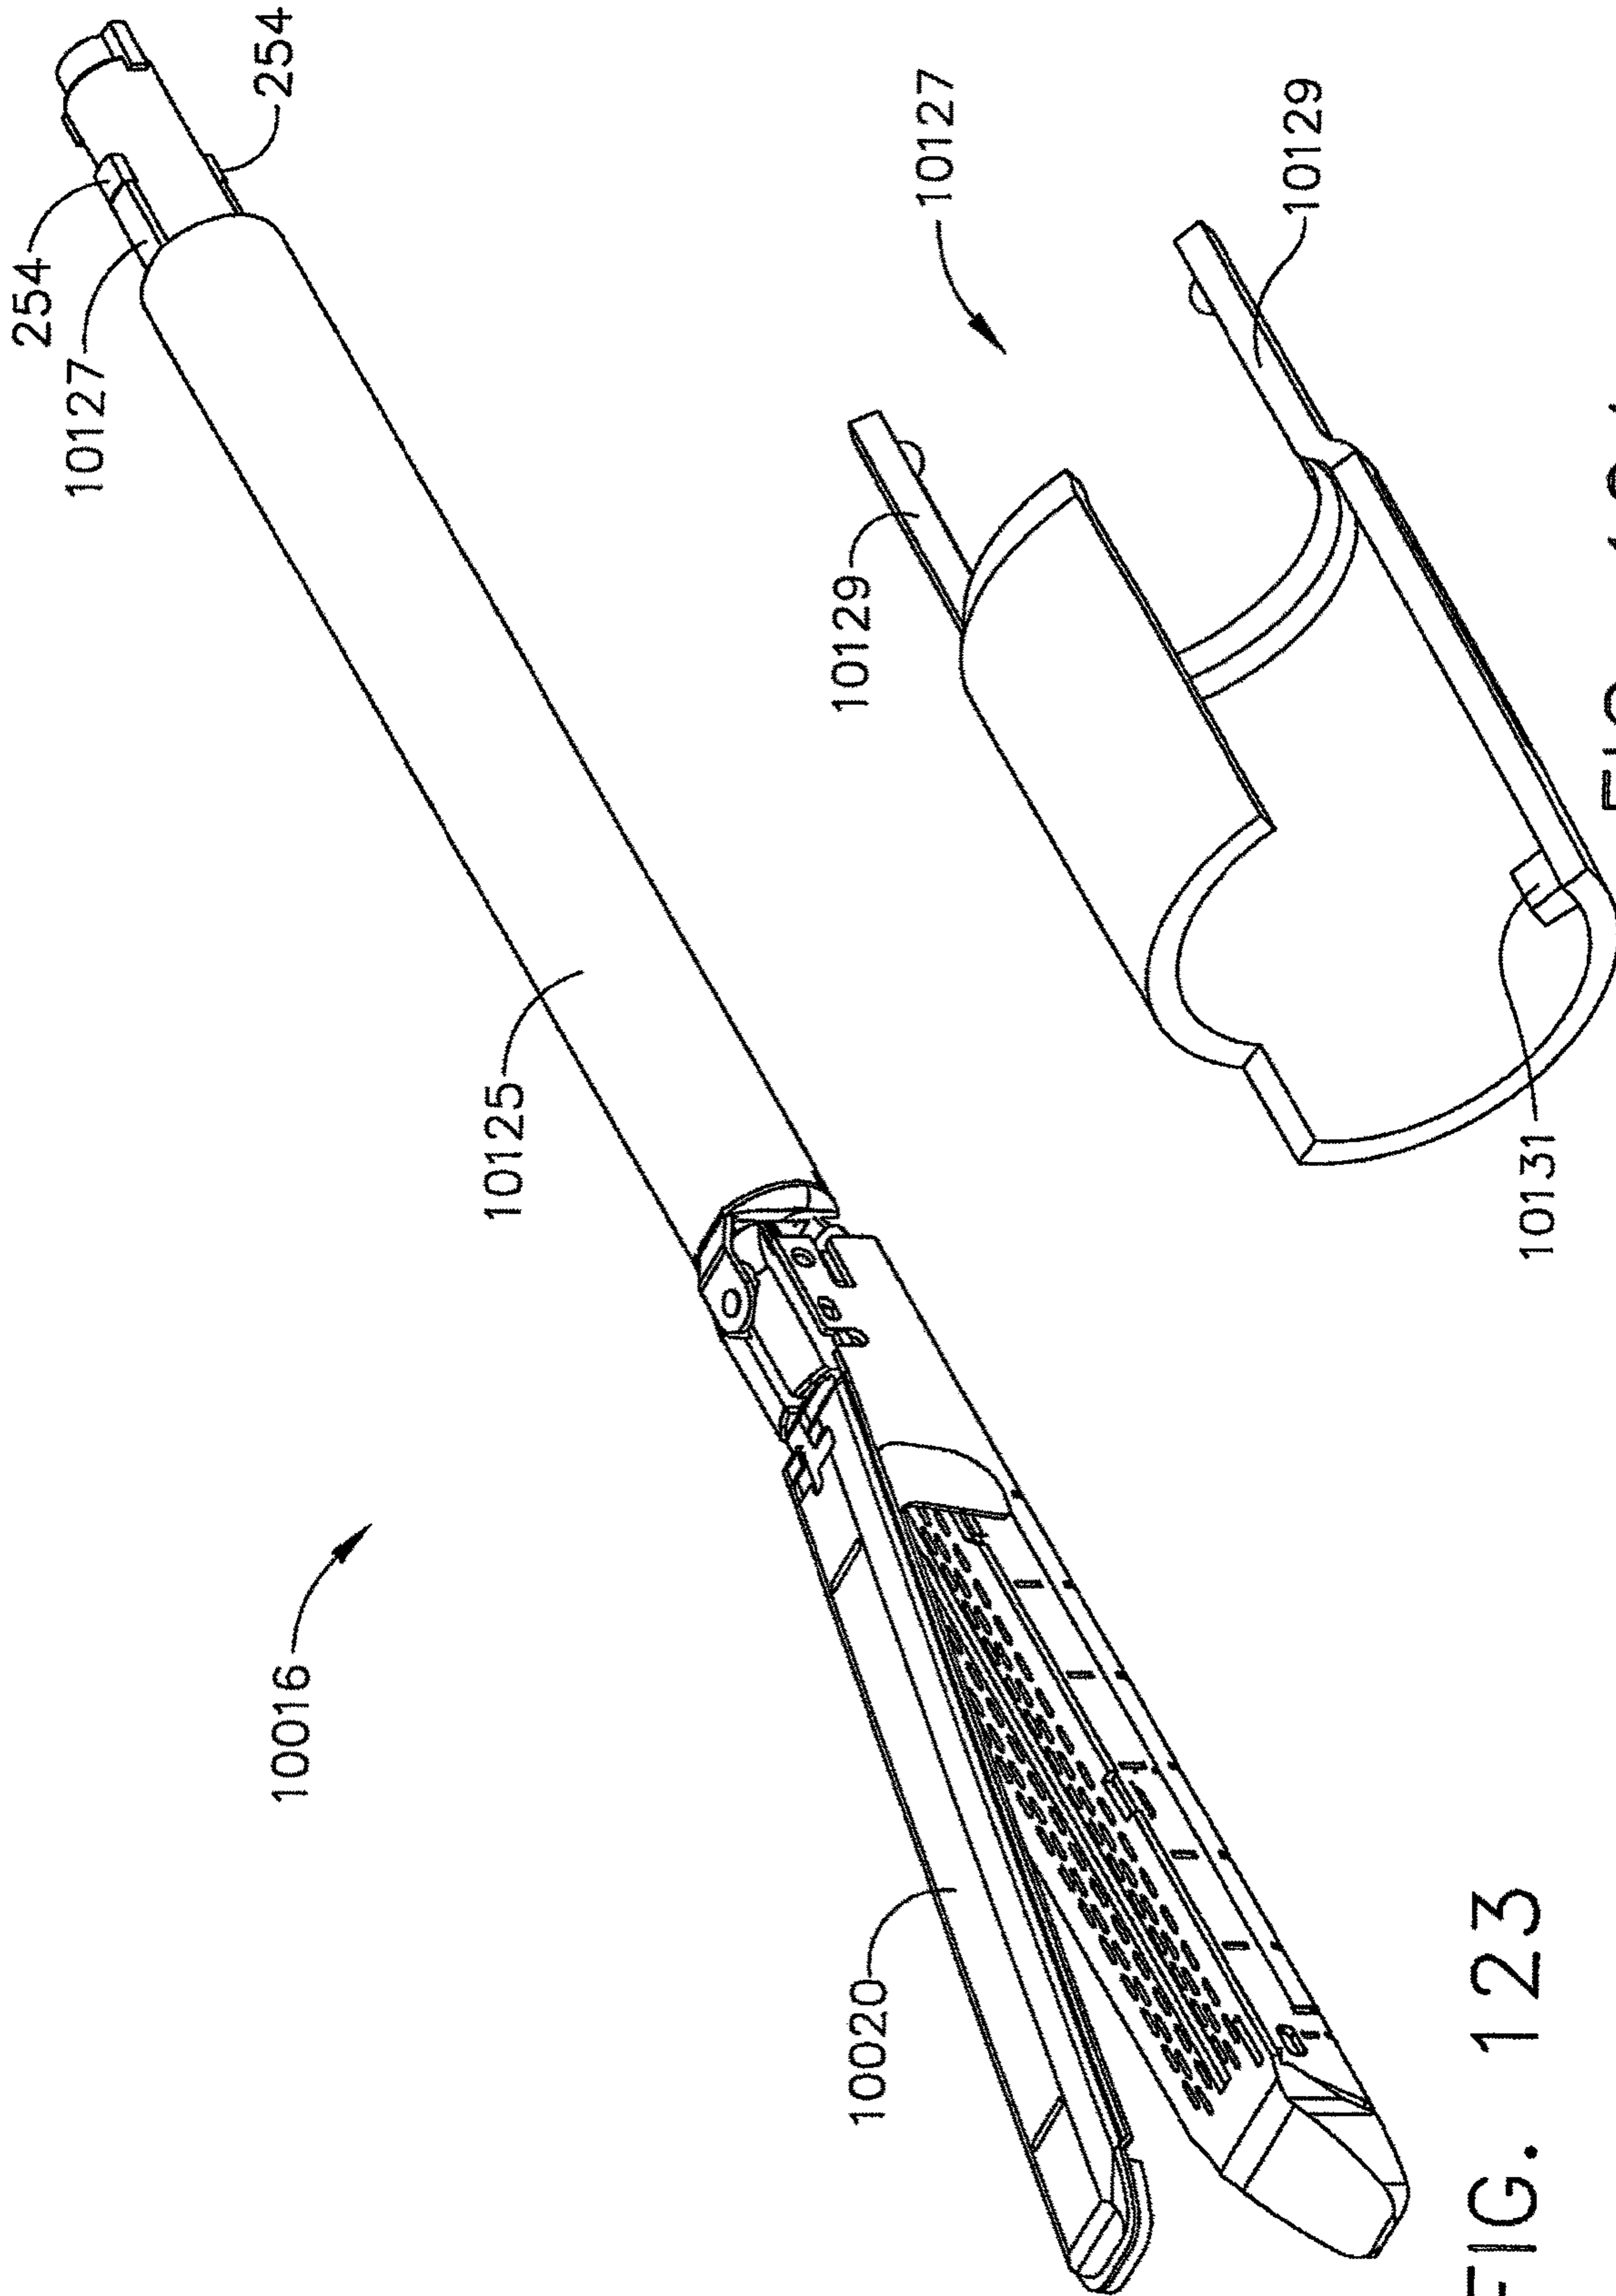


FIG. 123

FIG. 124

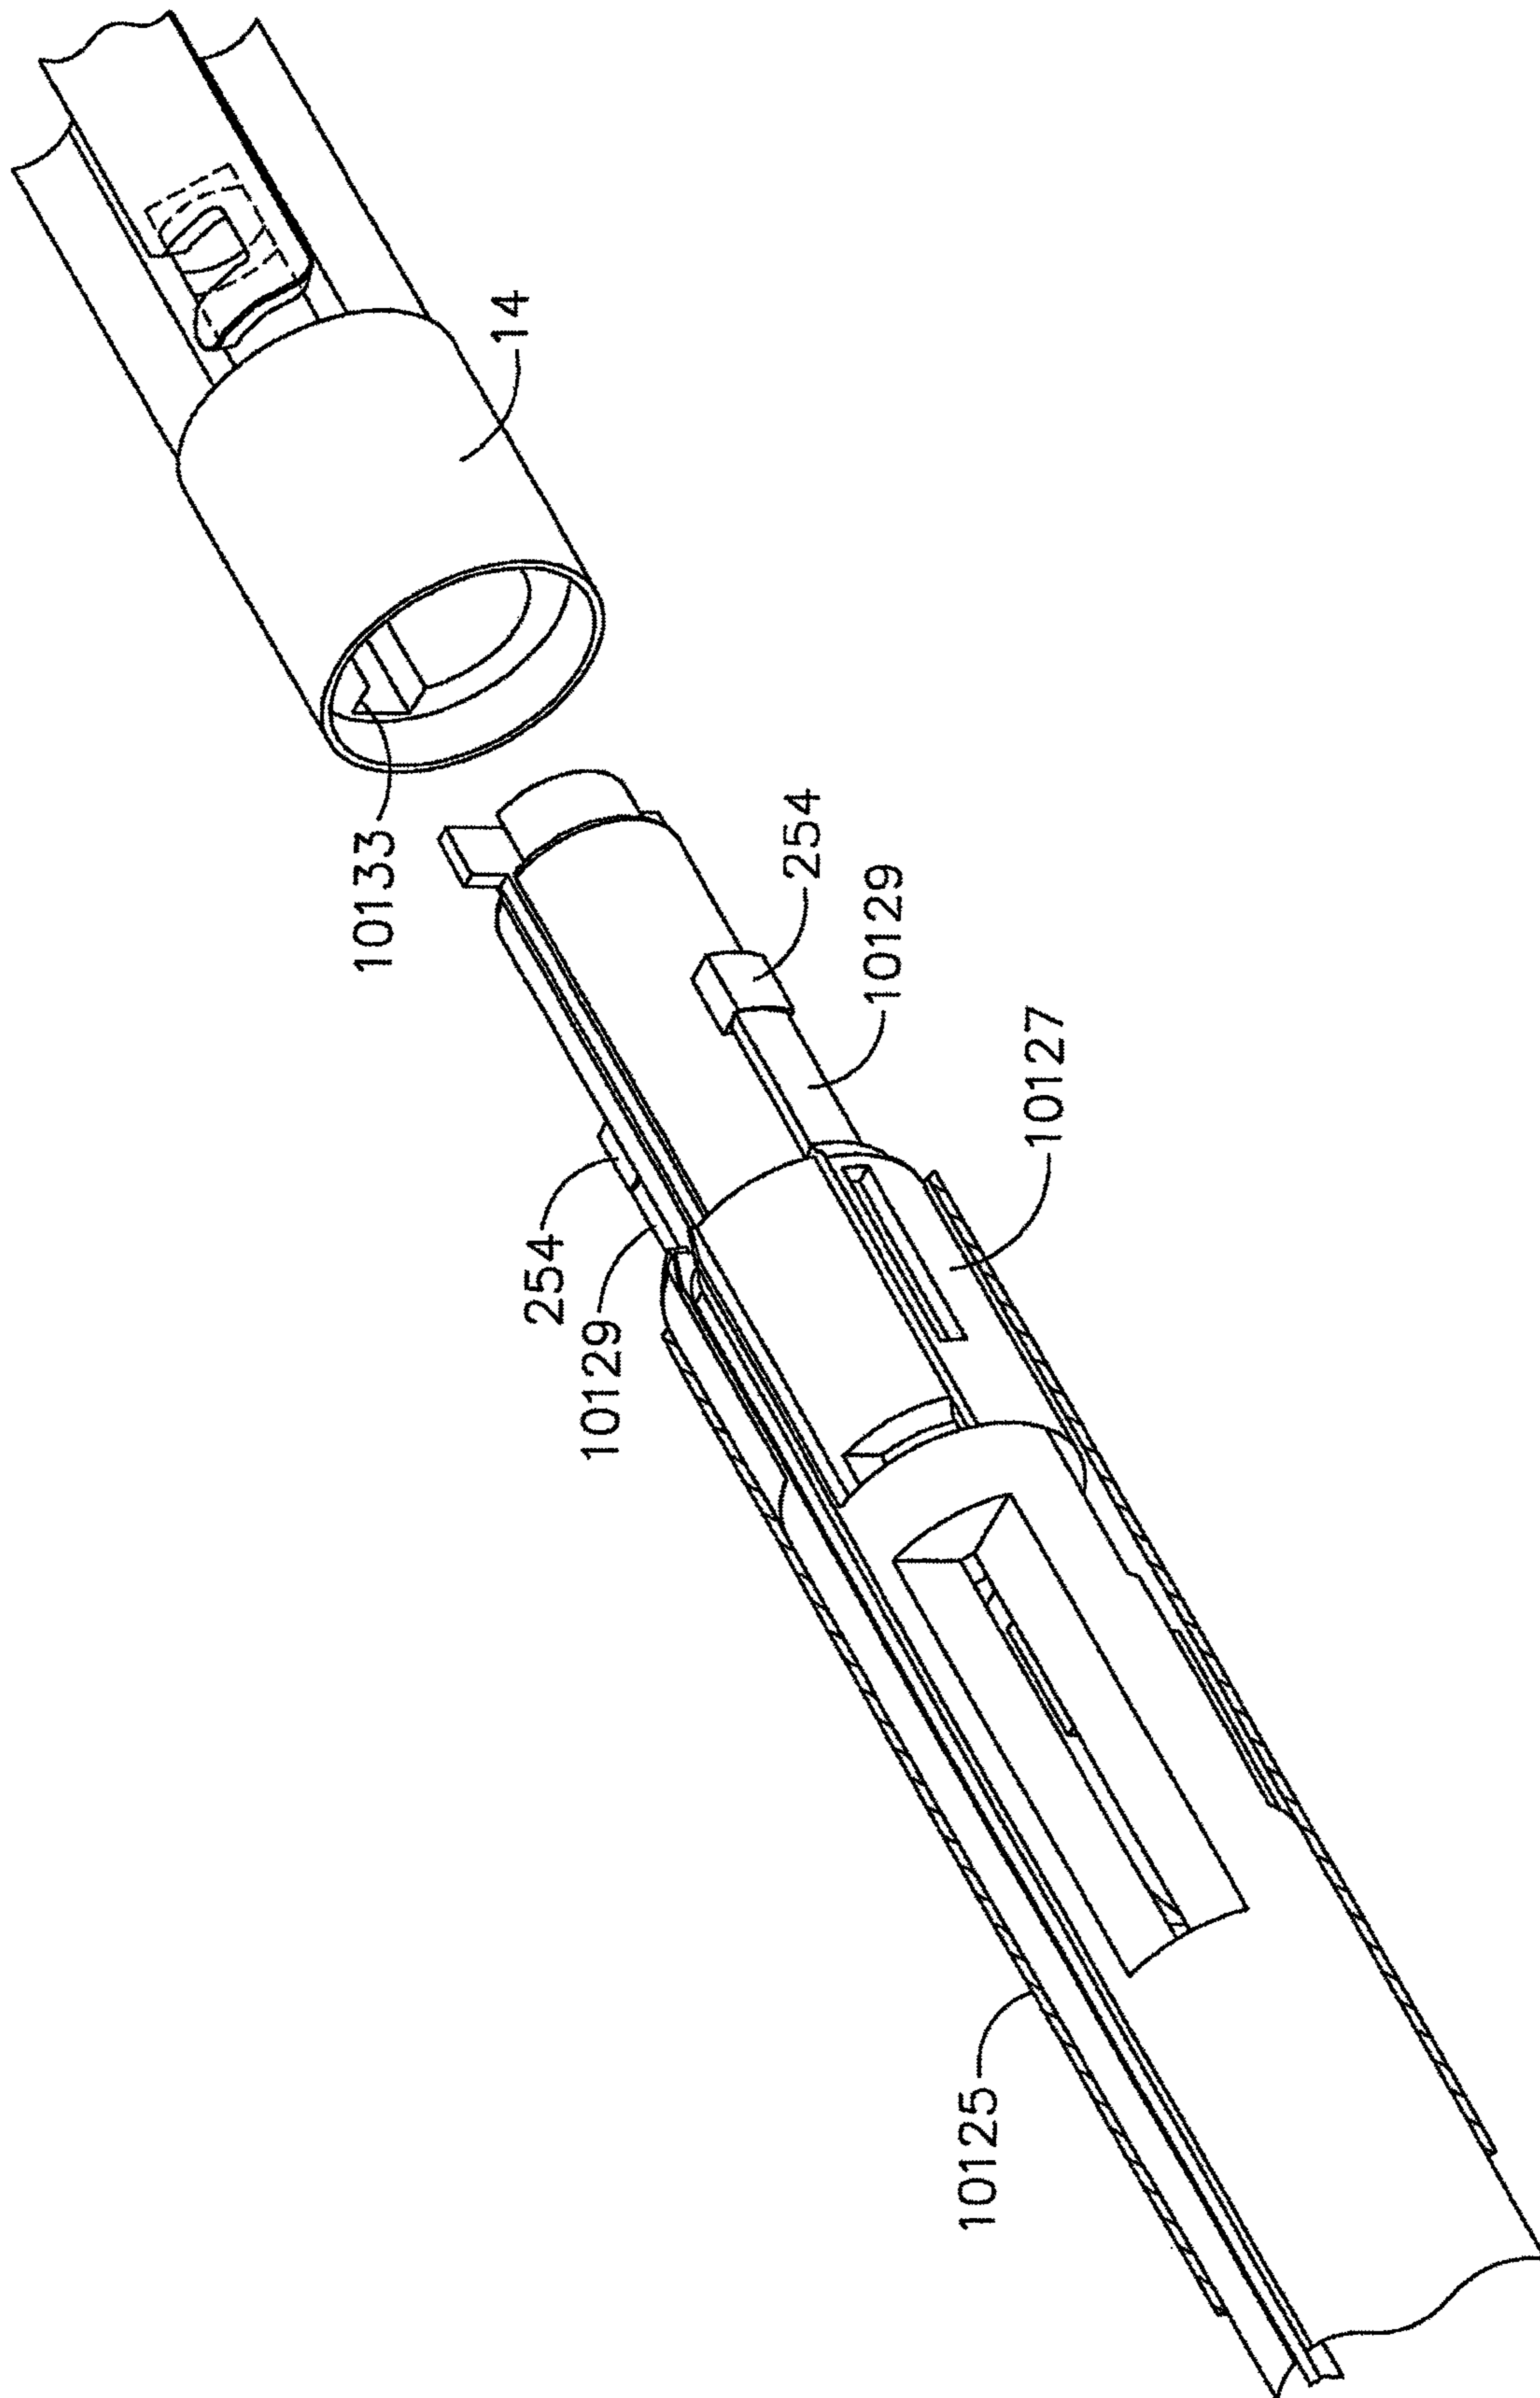


FIG. 125

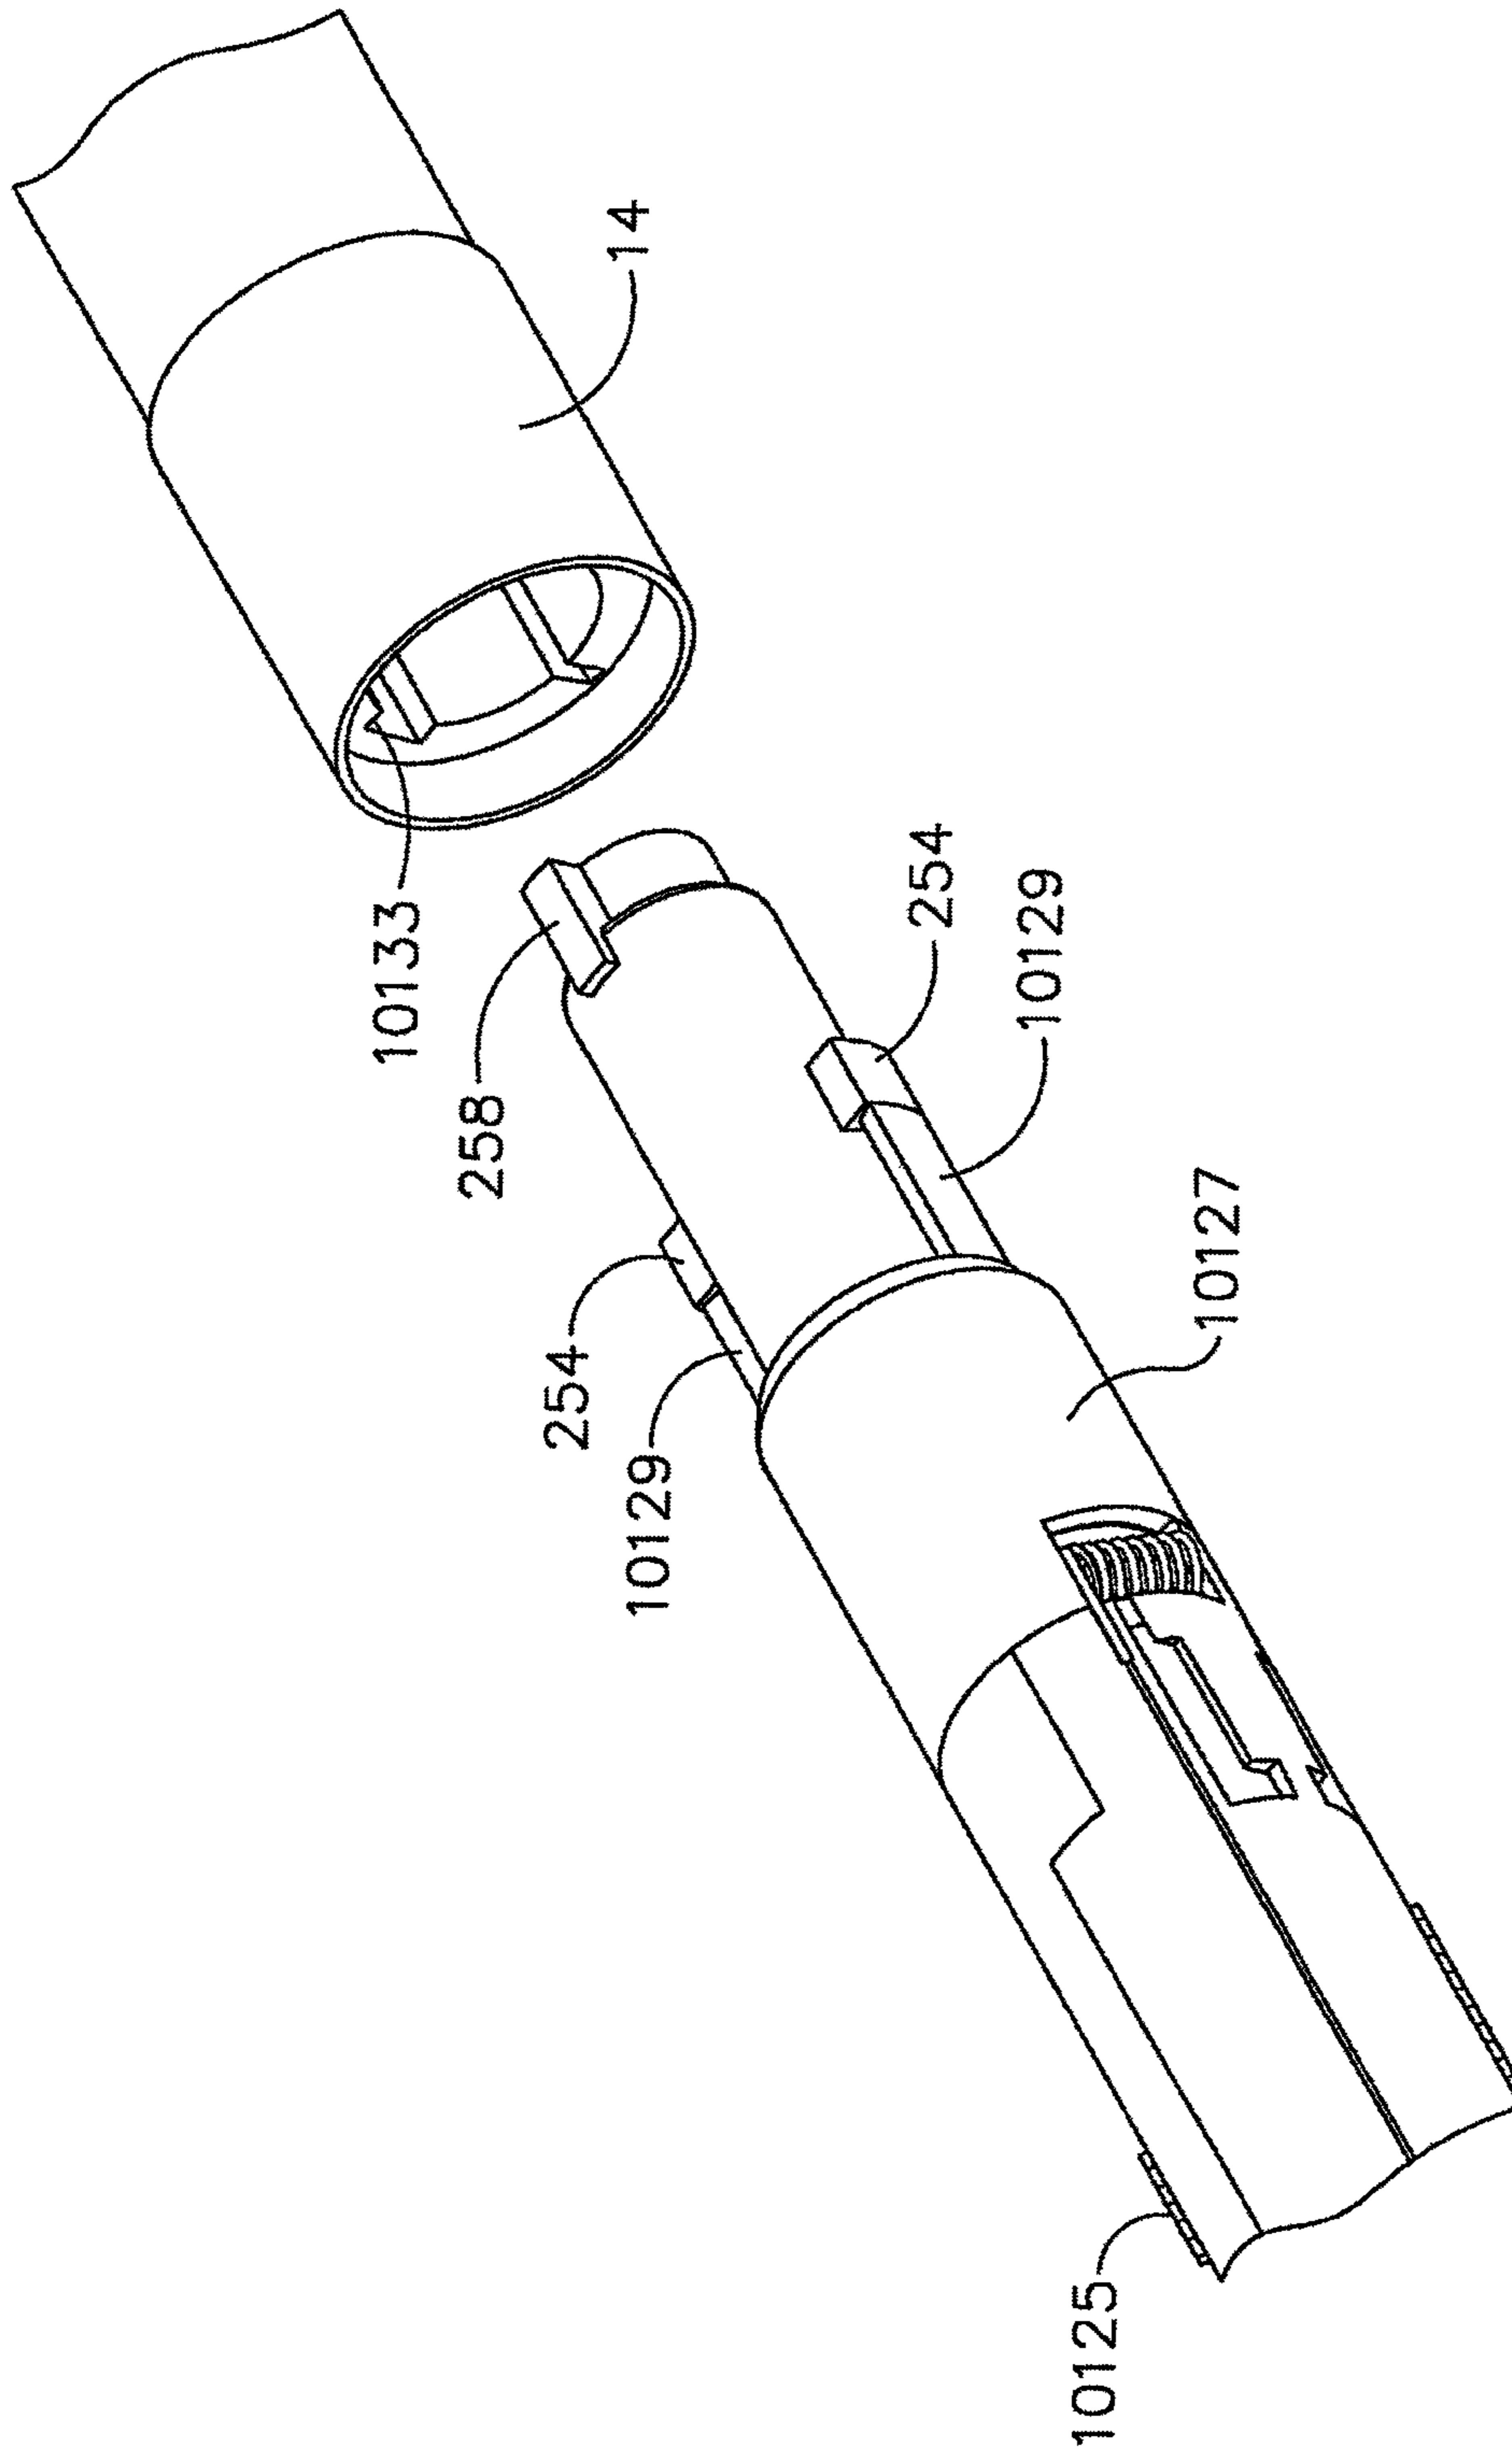


FIG. 126



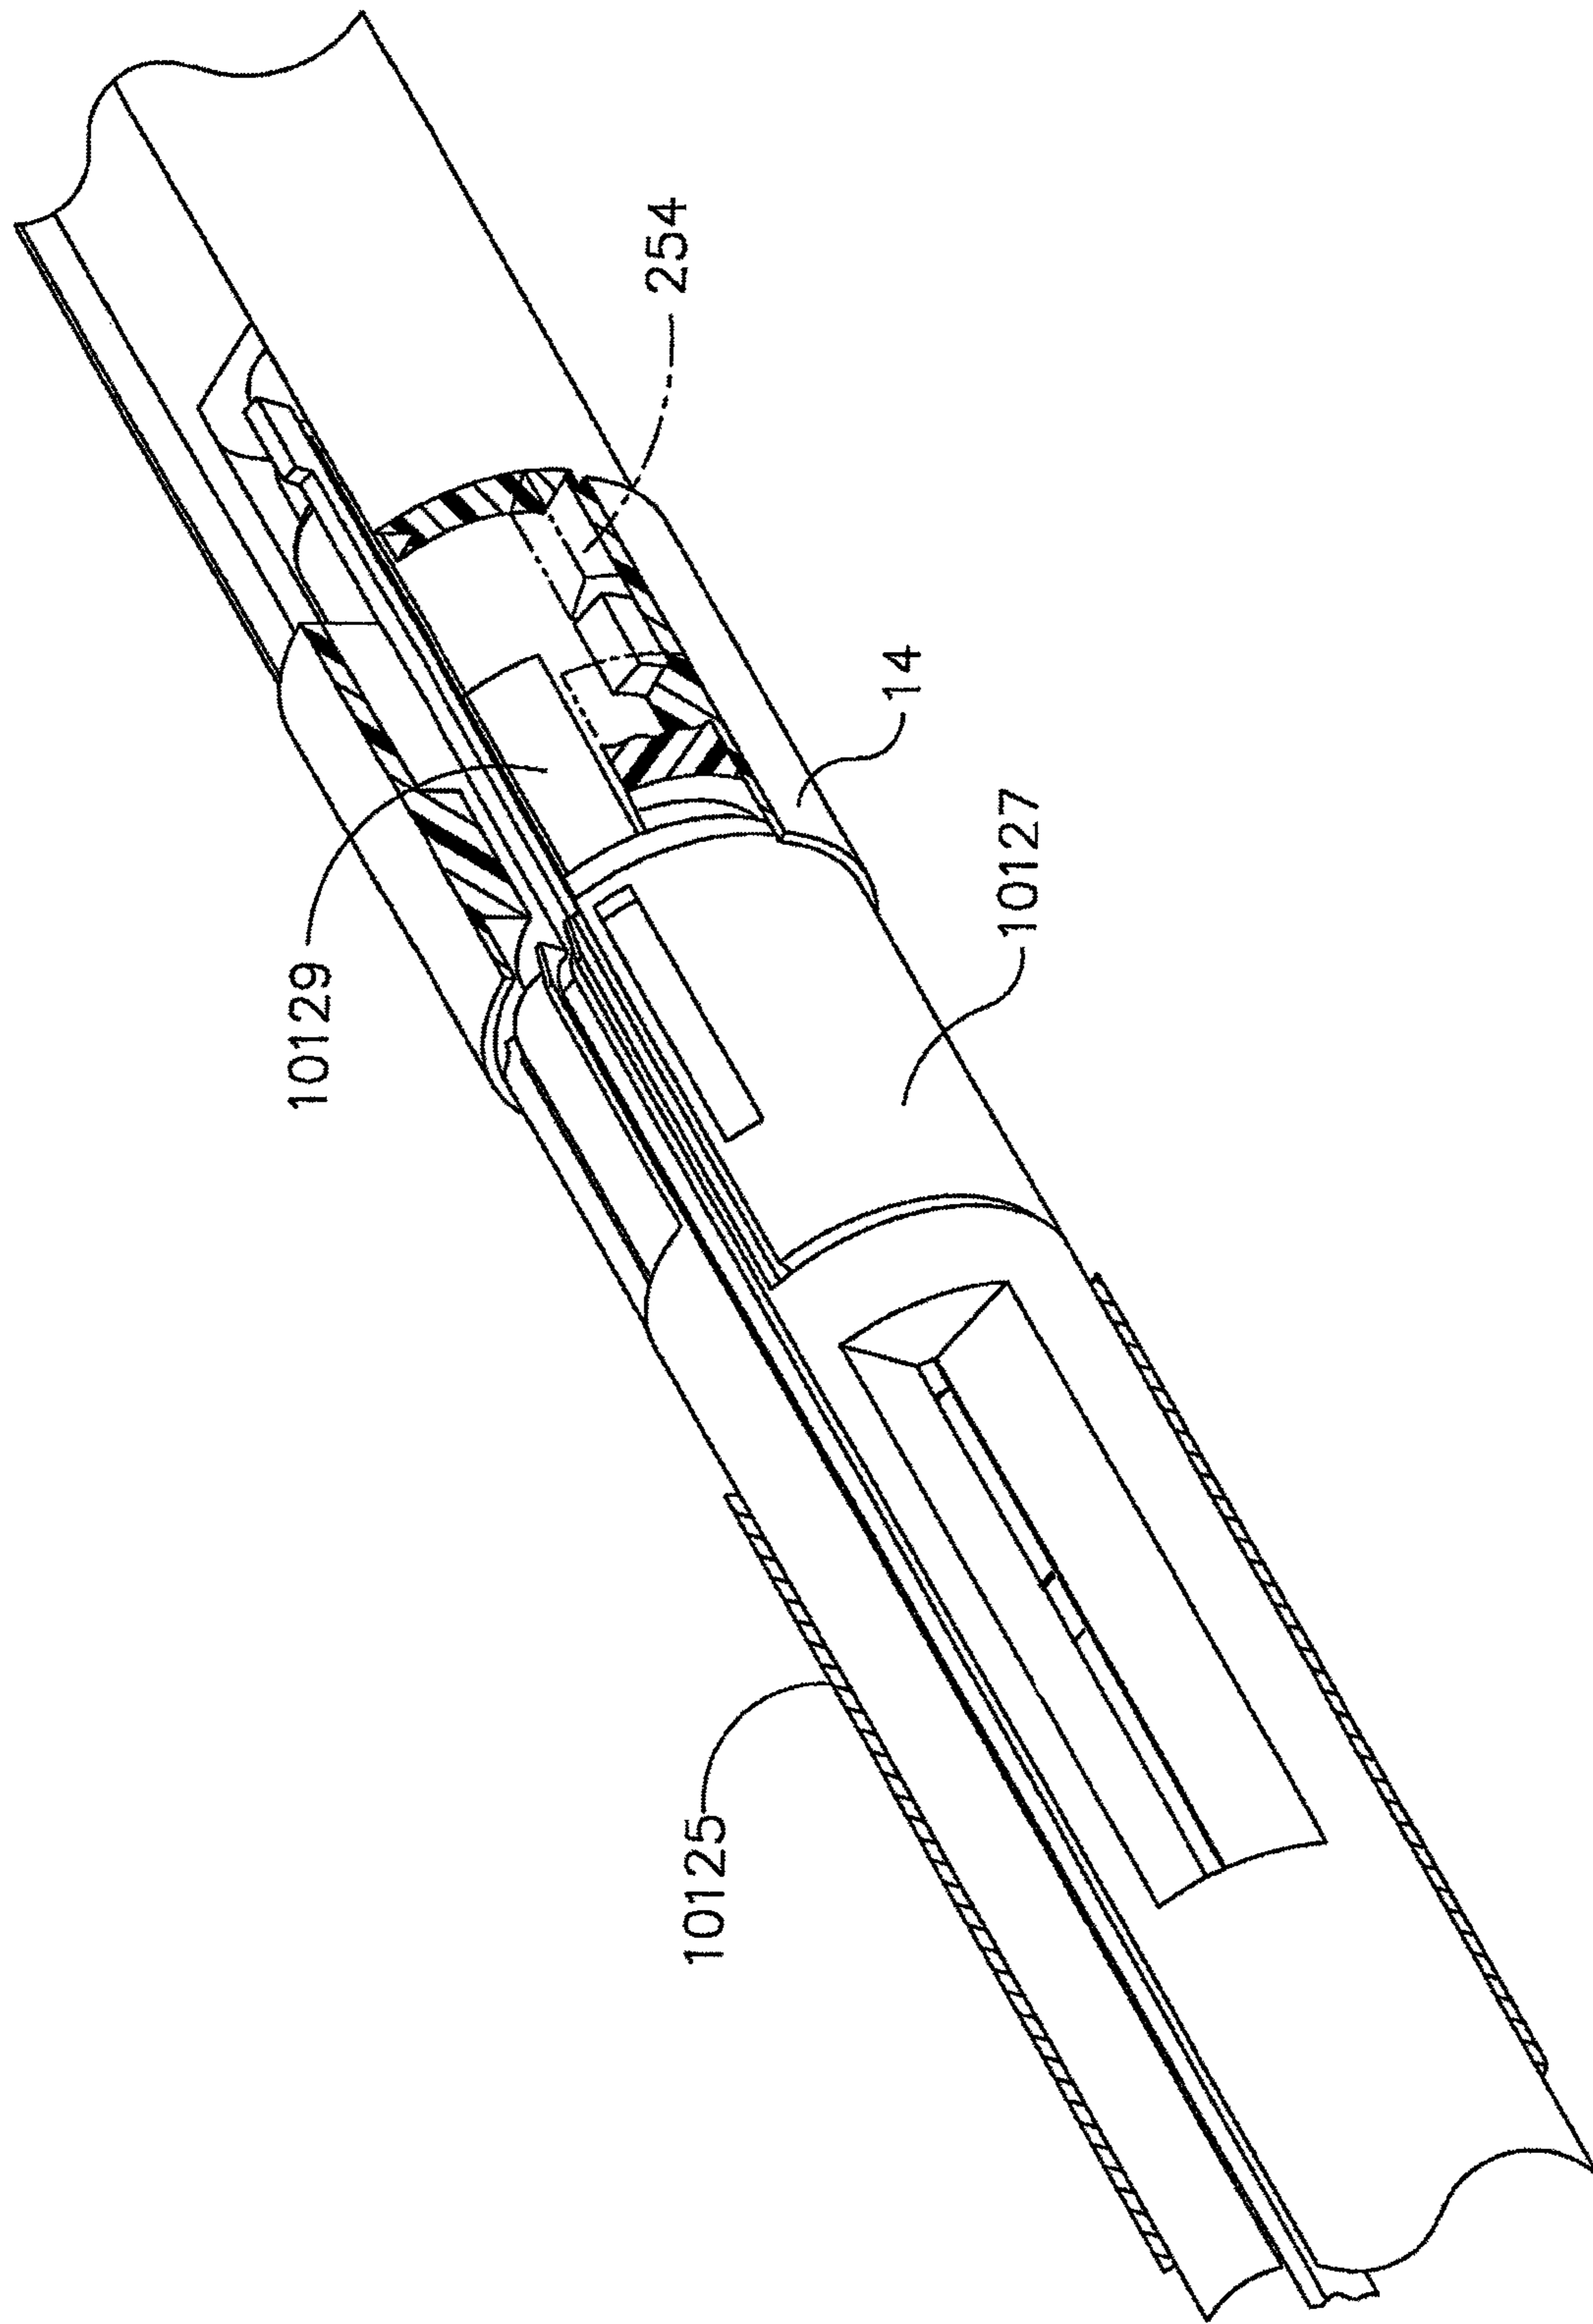


FIG. 127

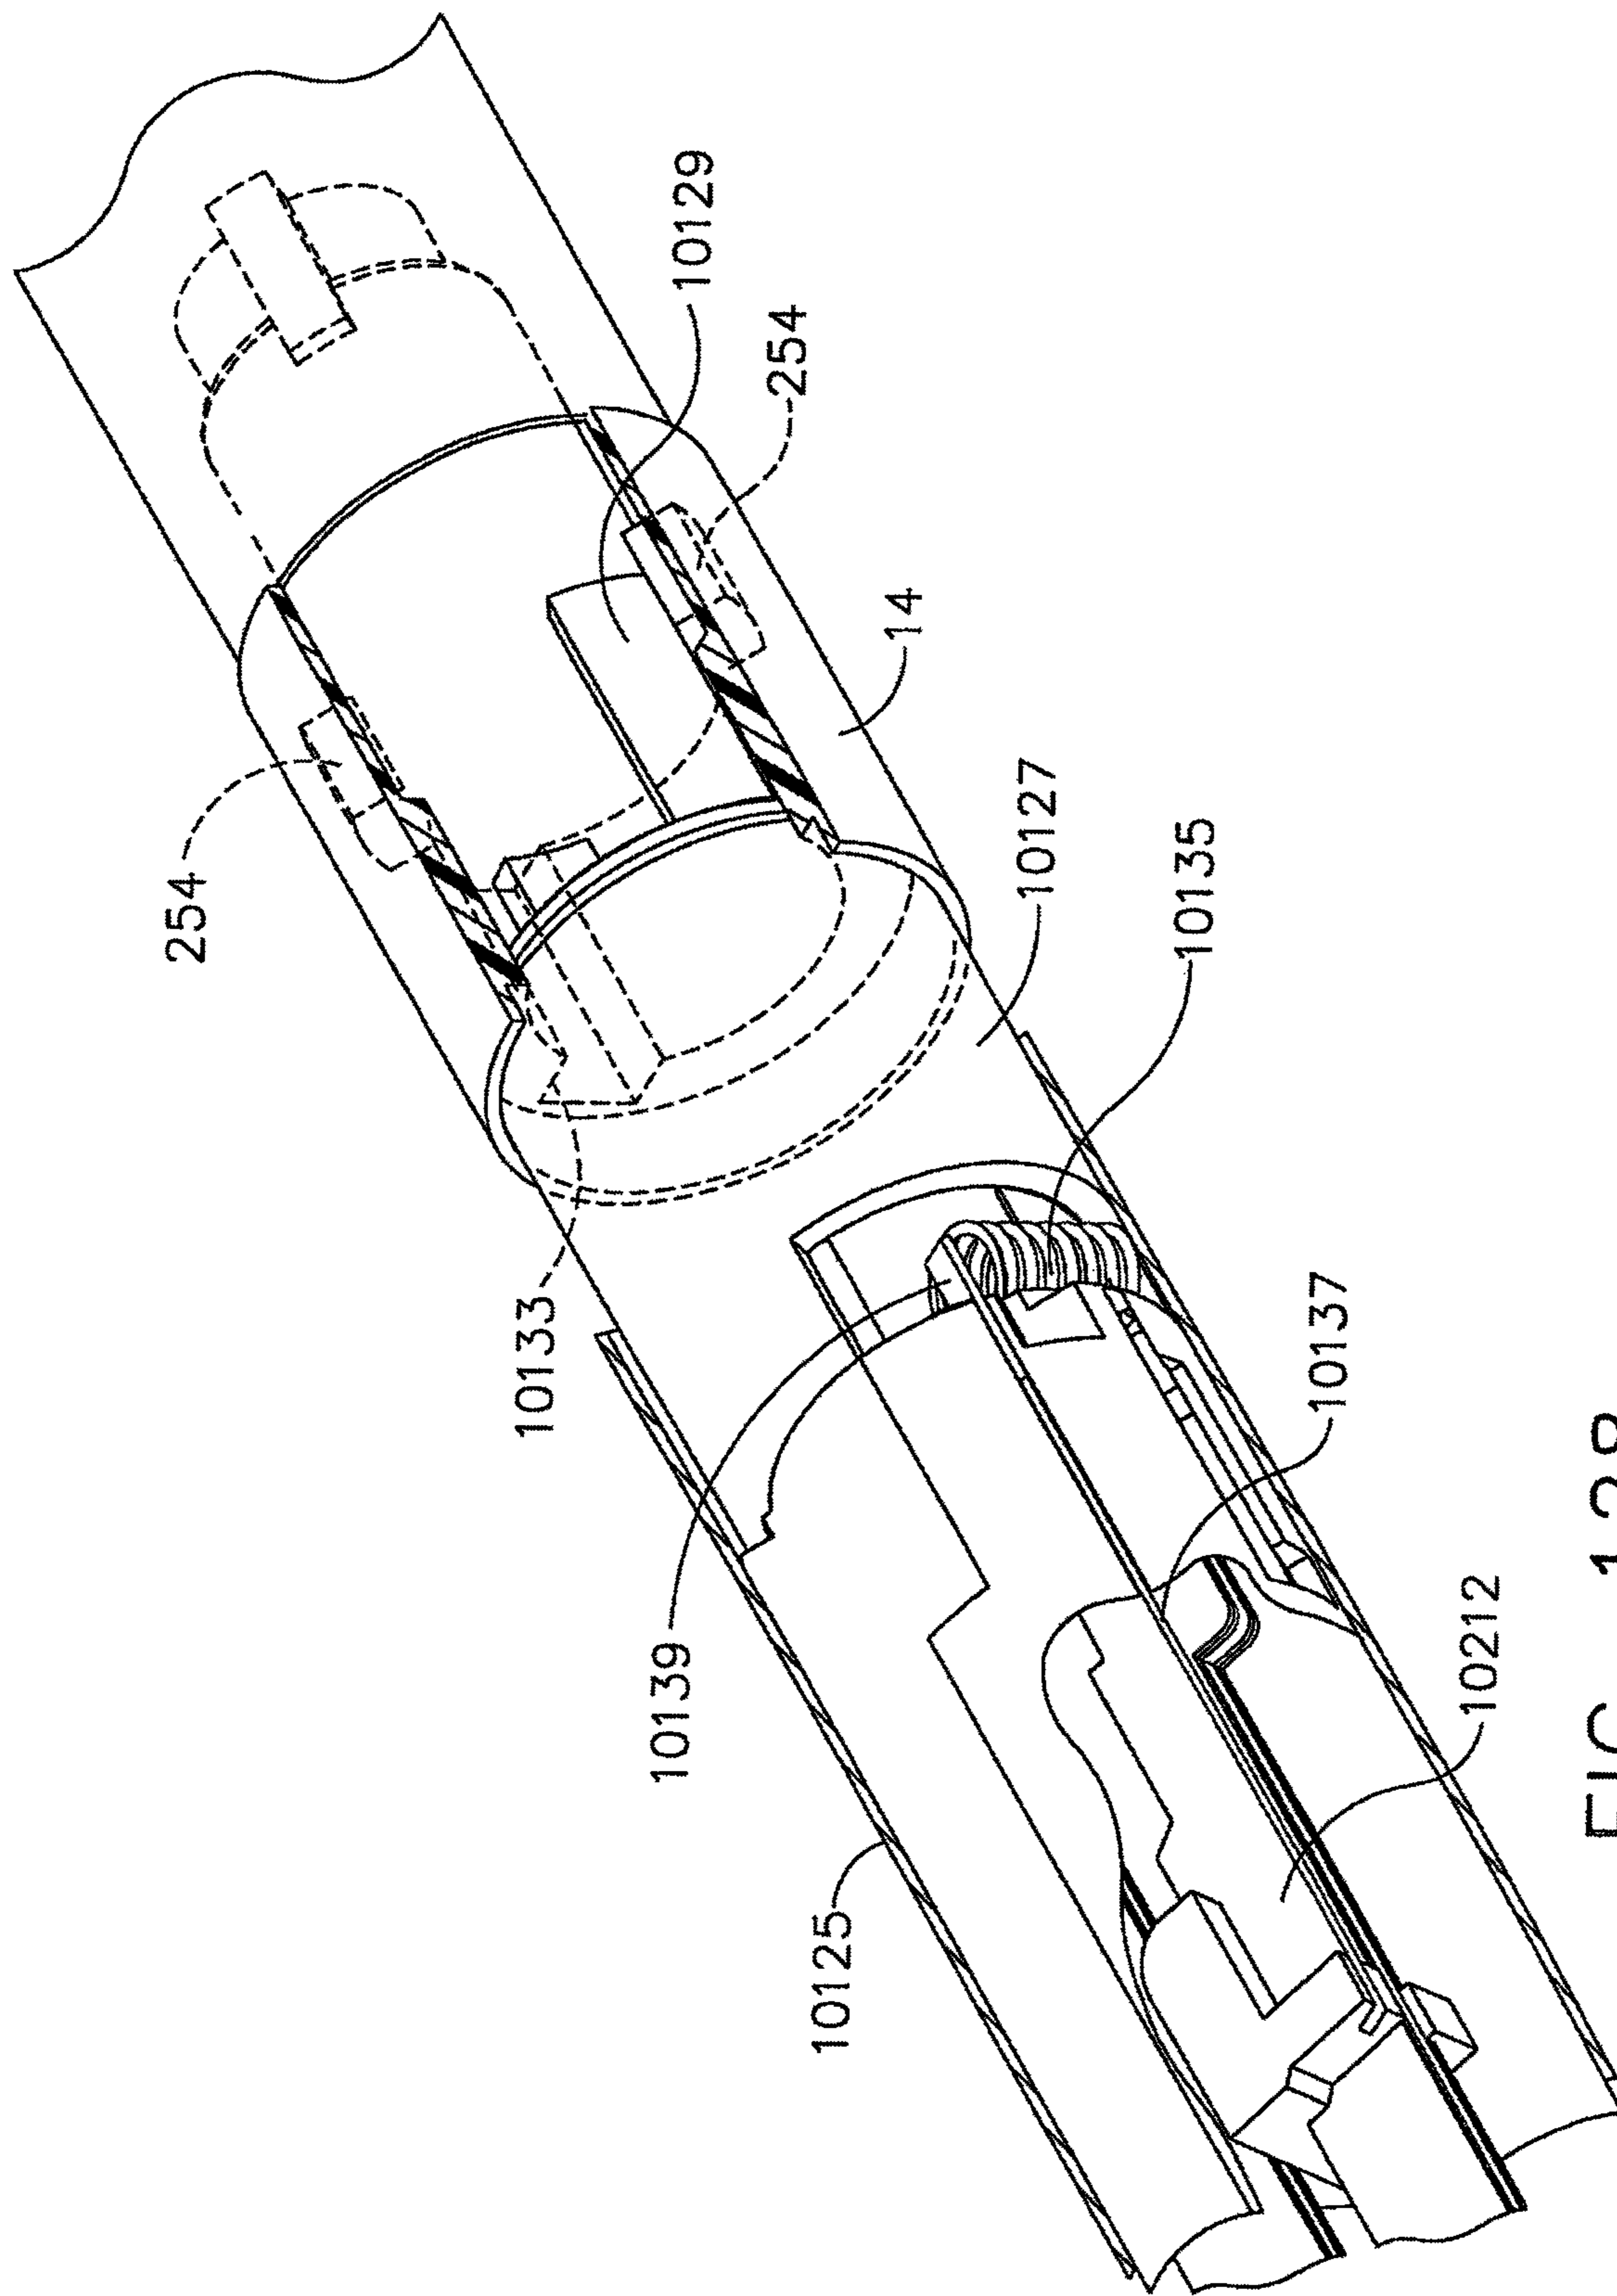


FIG. 128

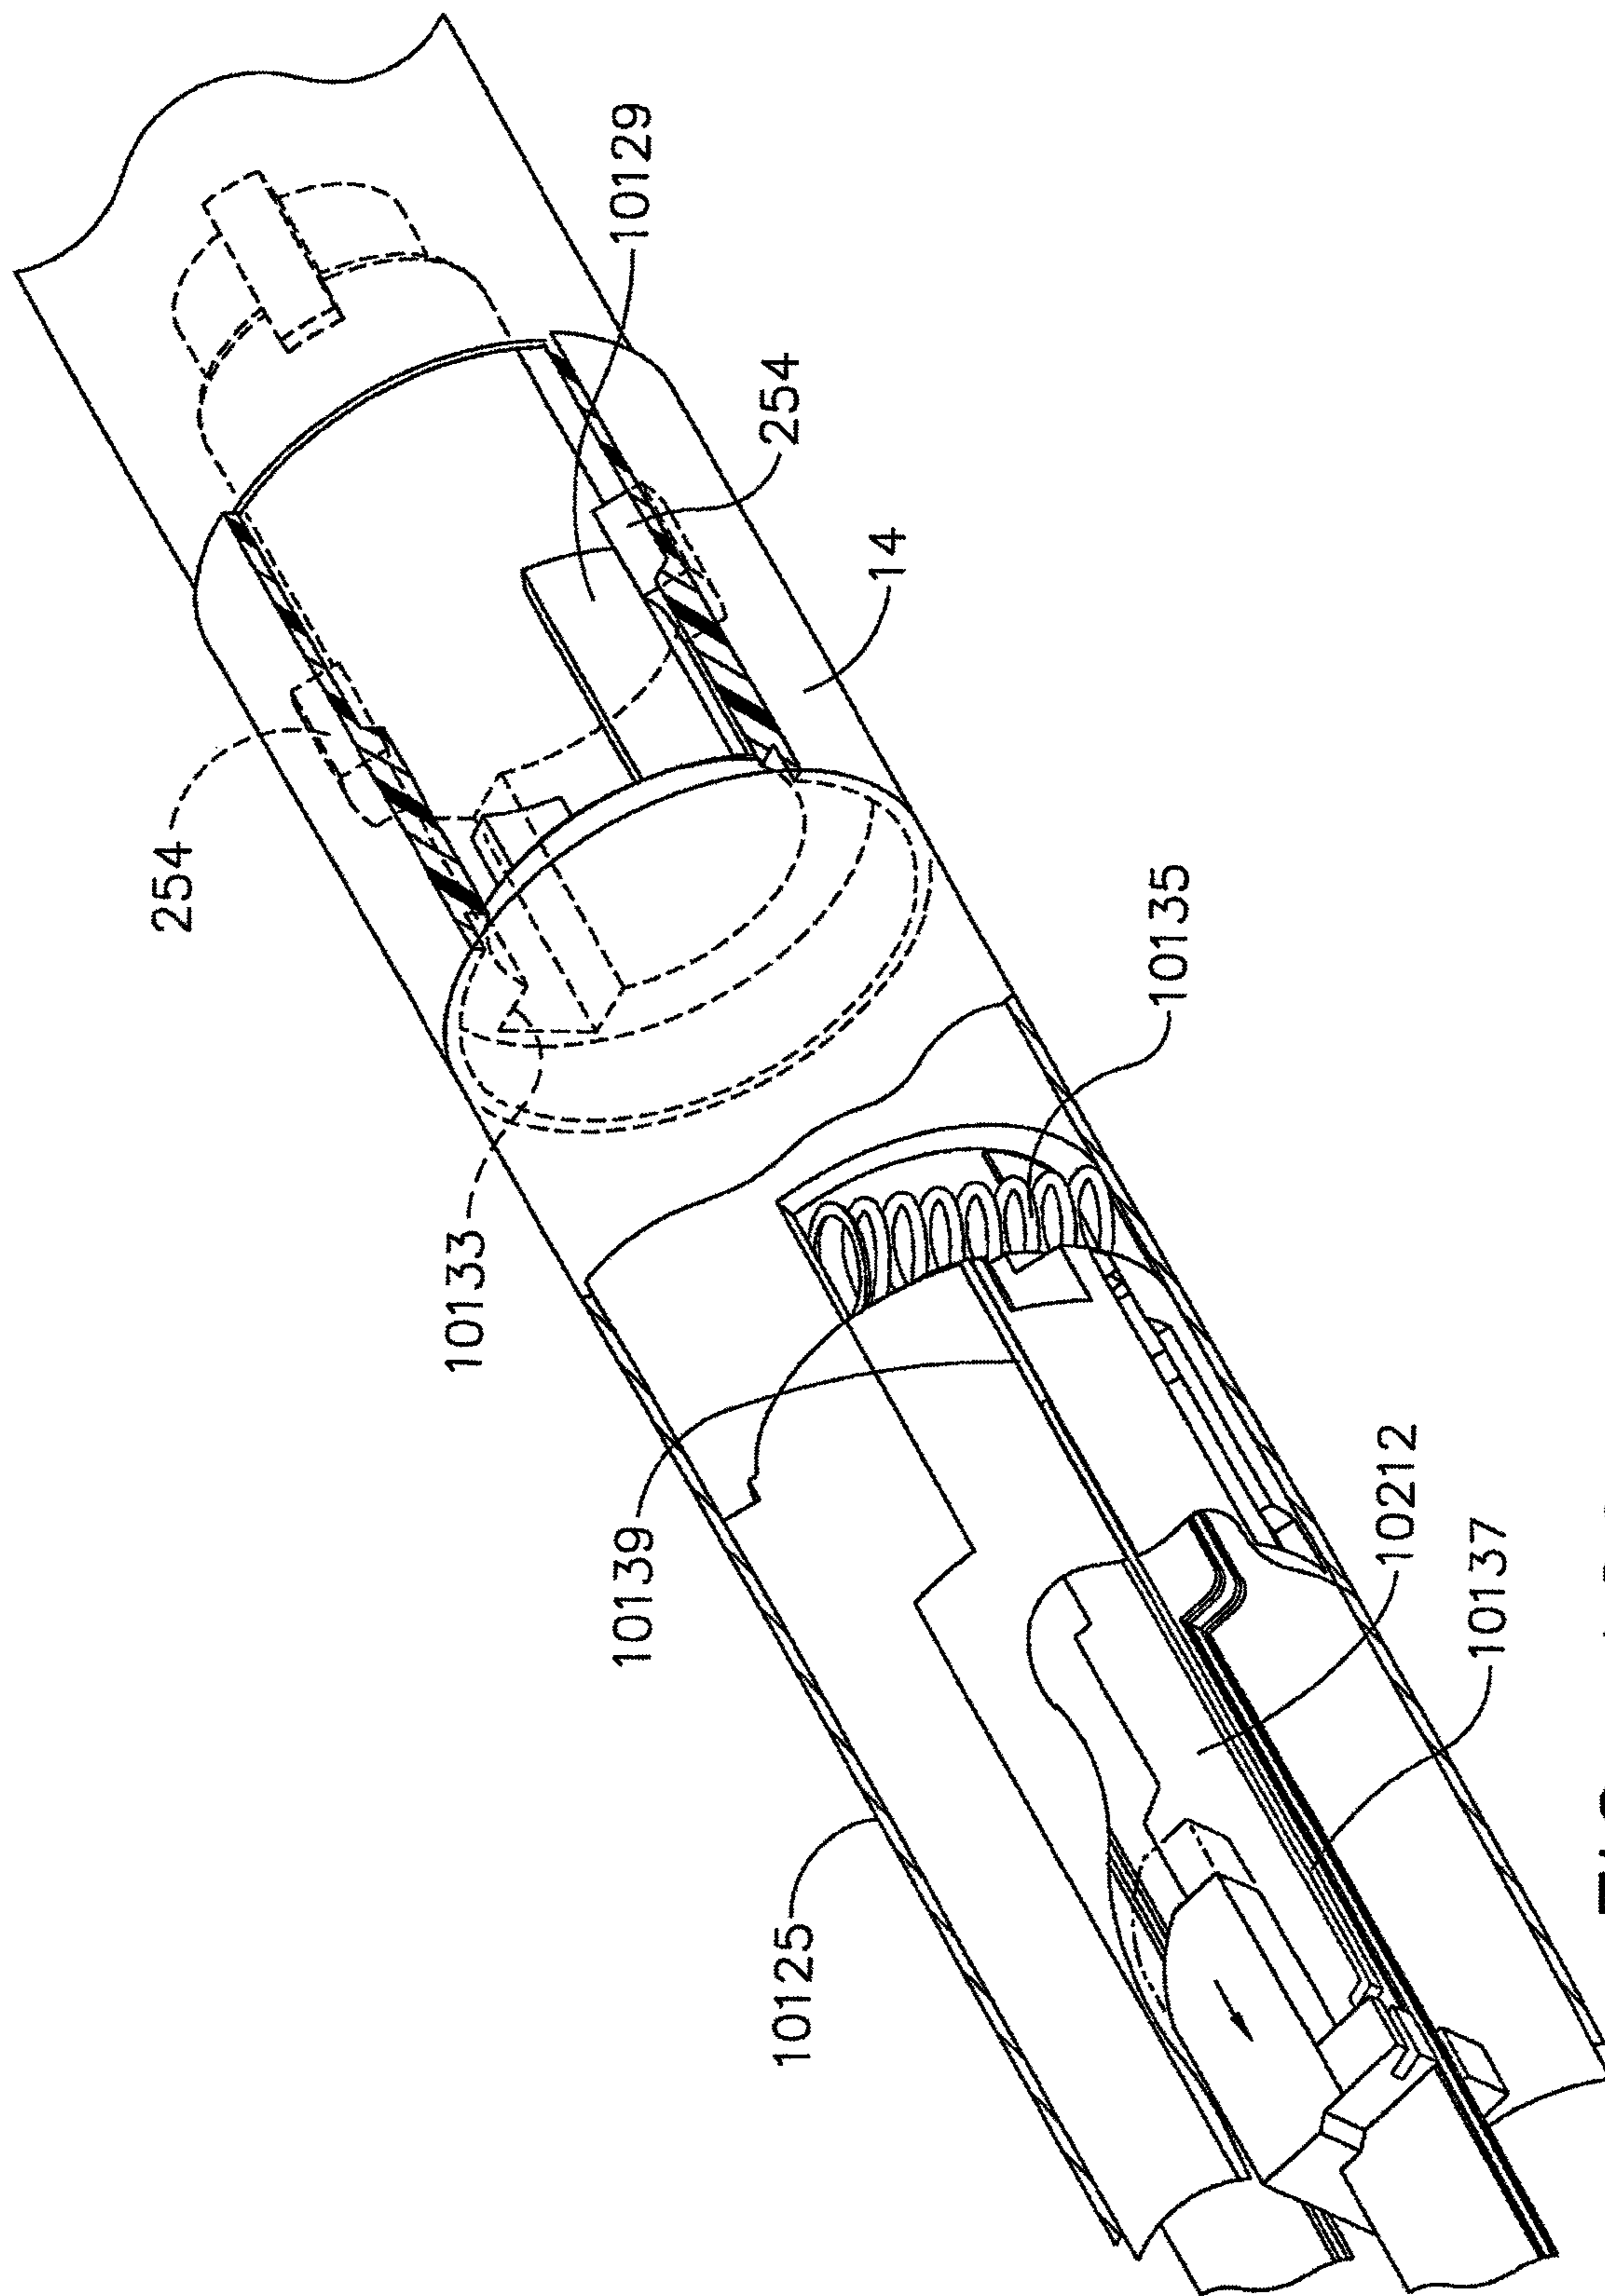


FIG. 129

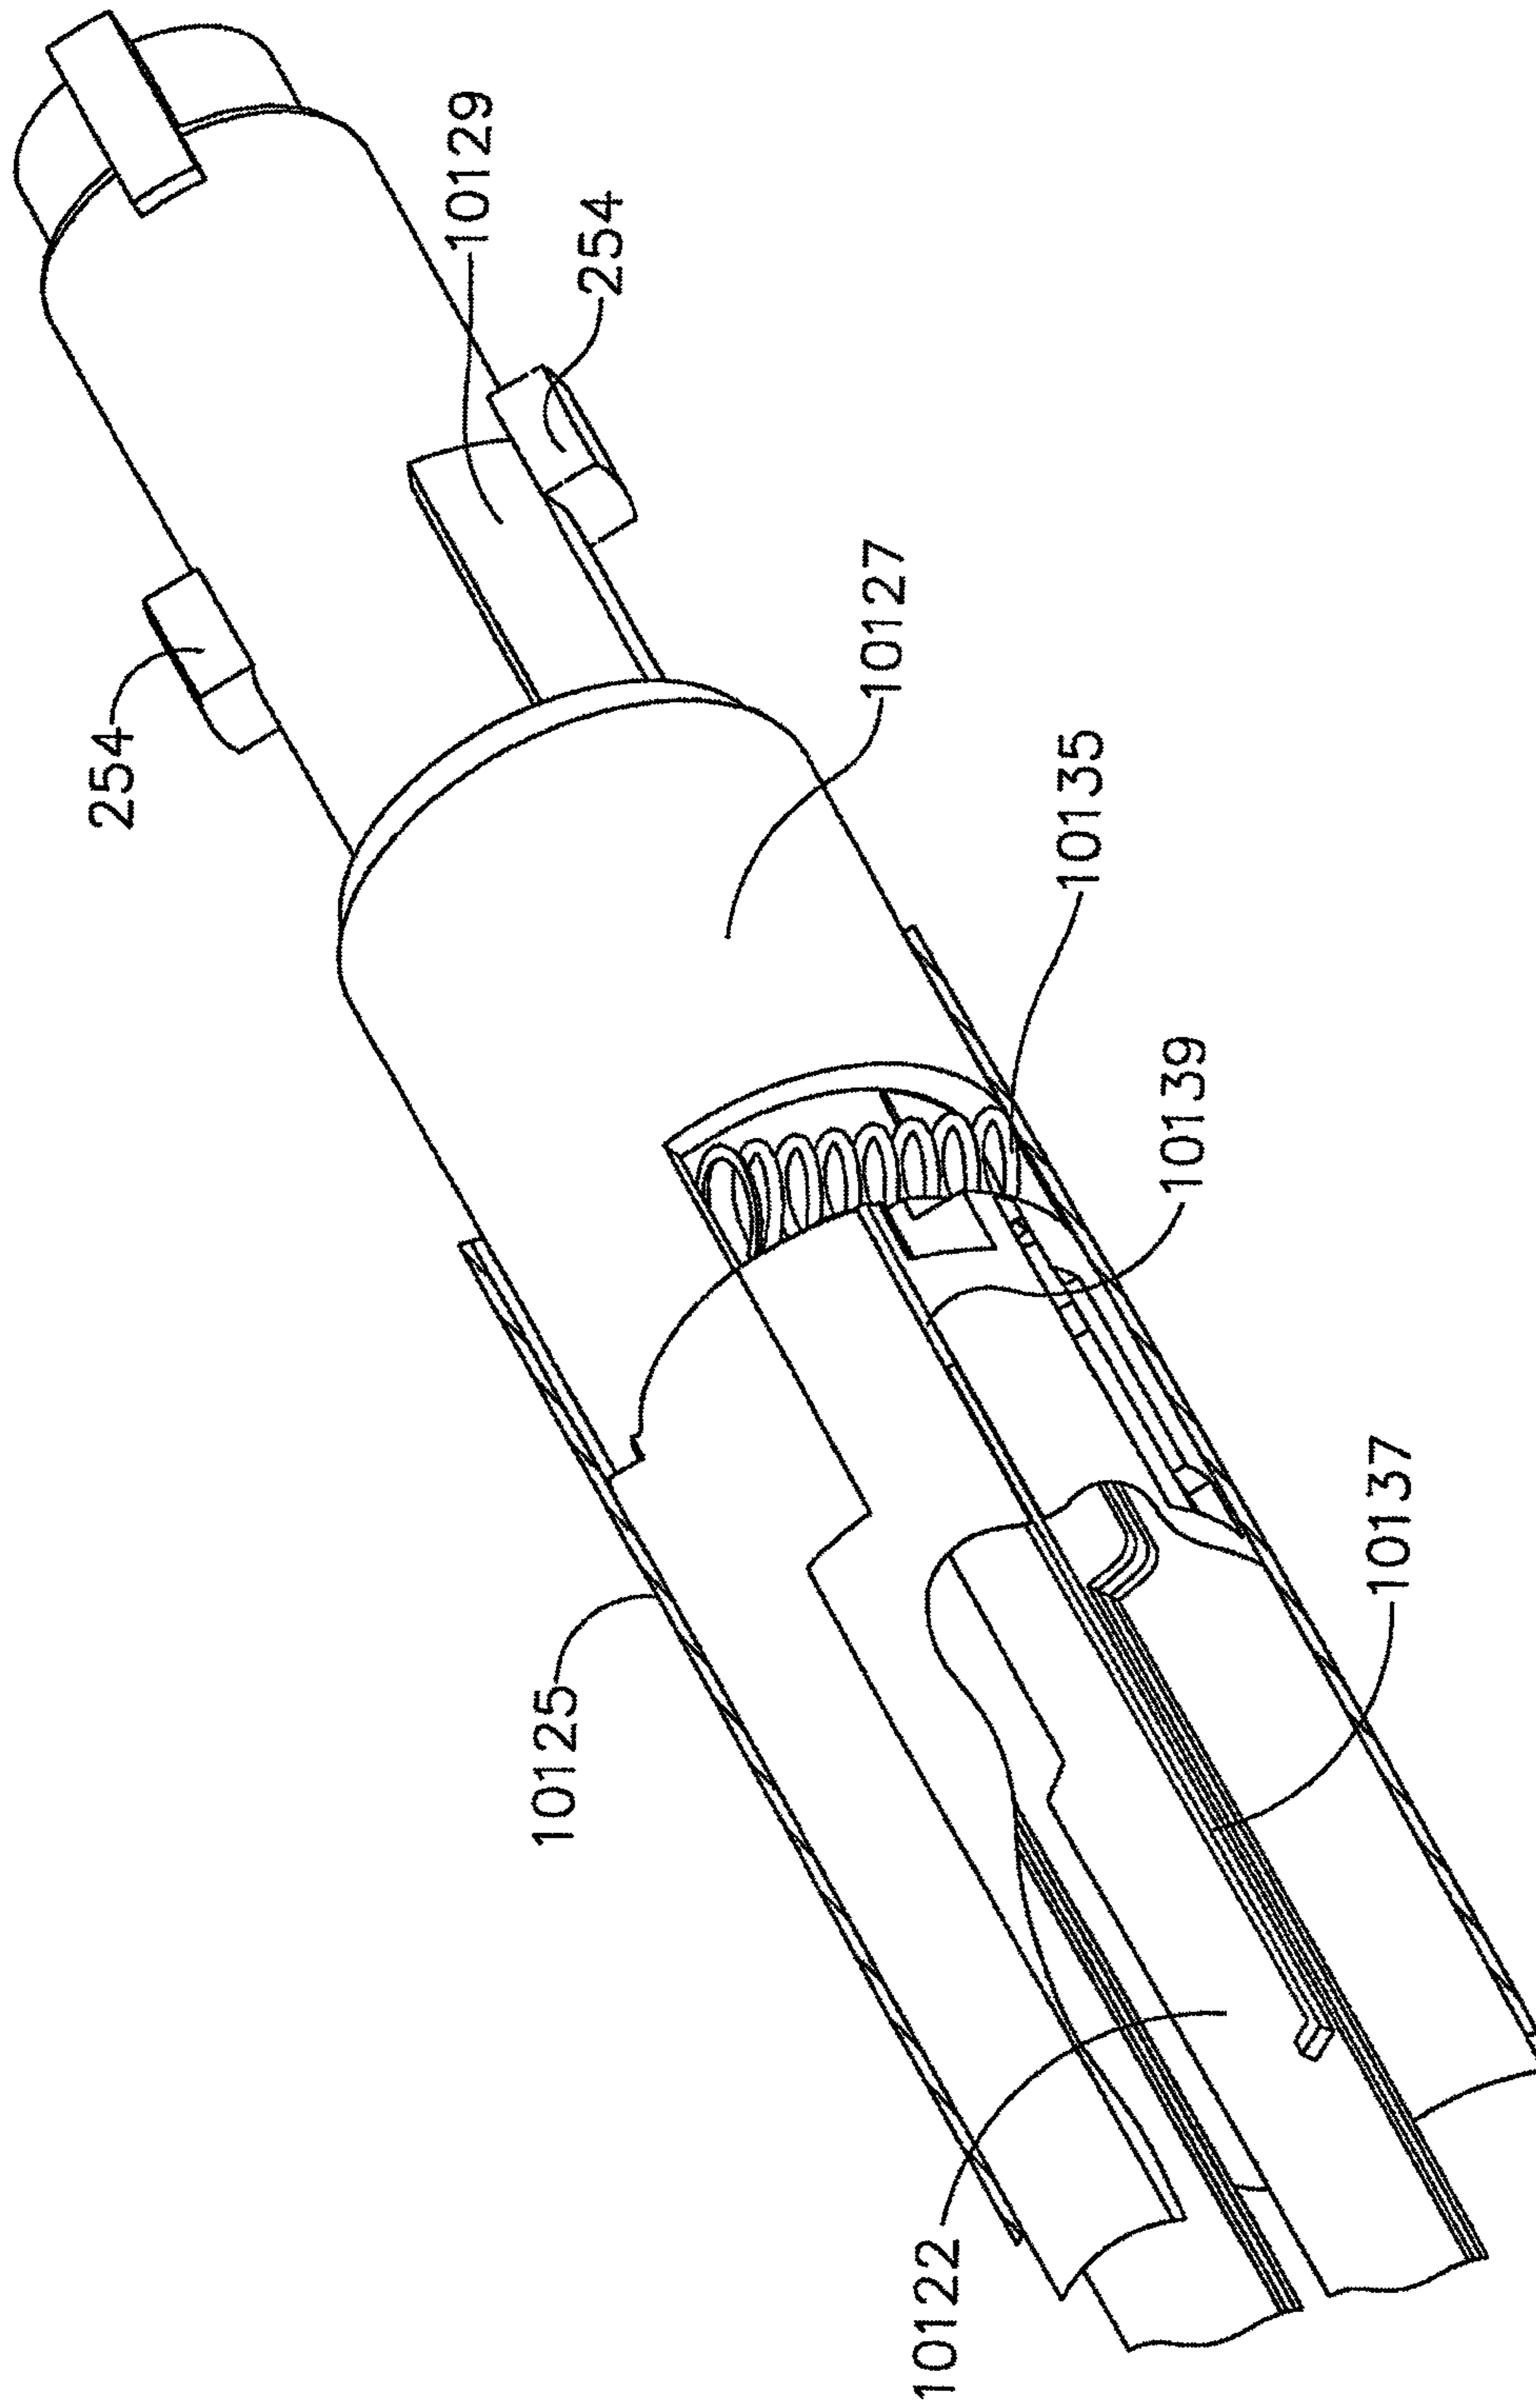


FIG. 130

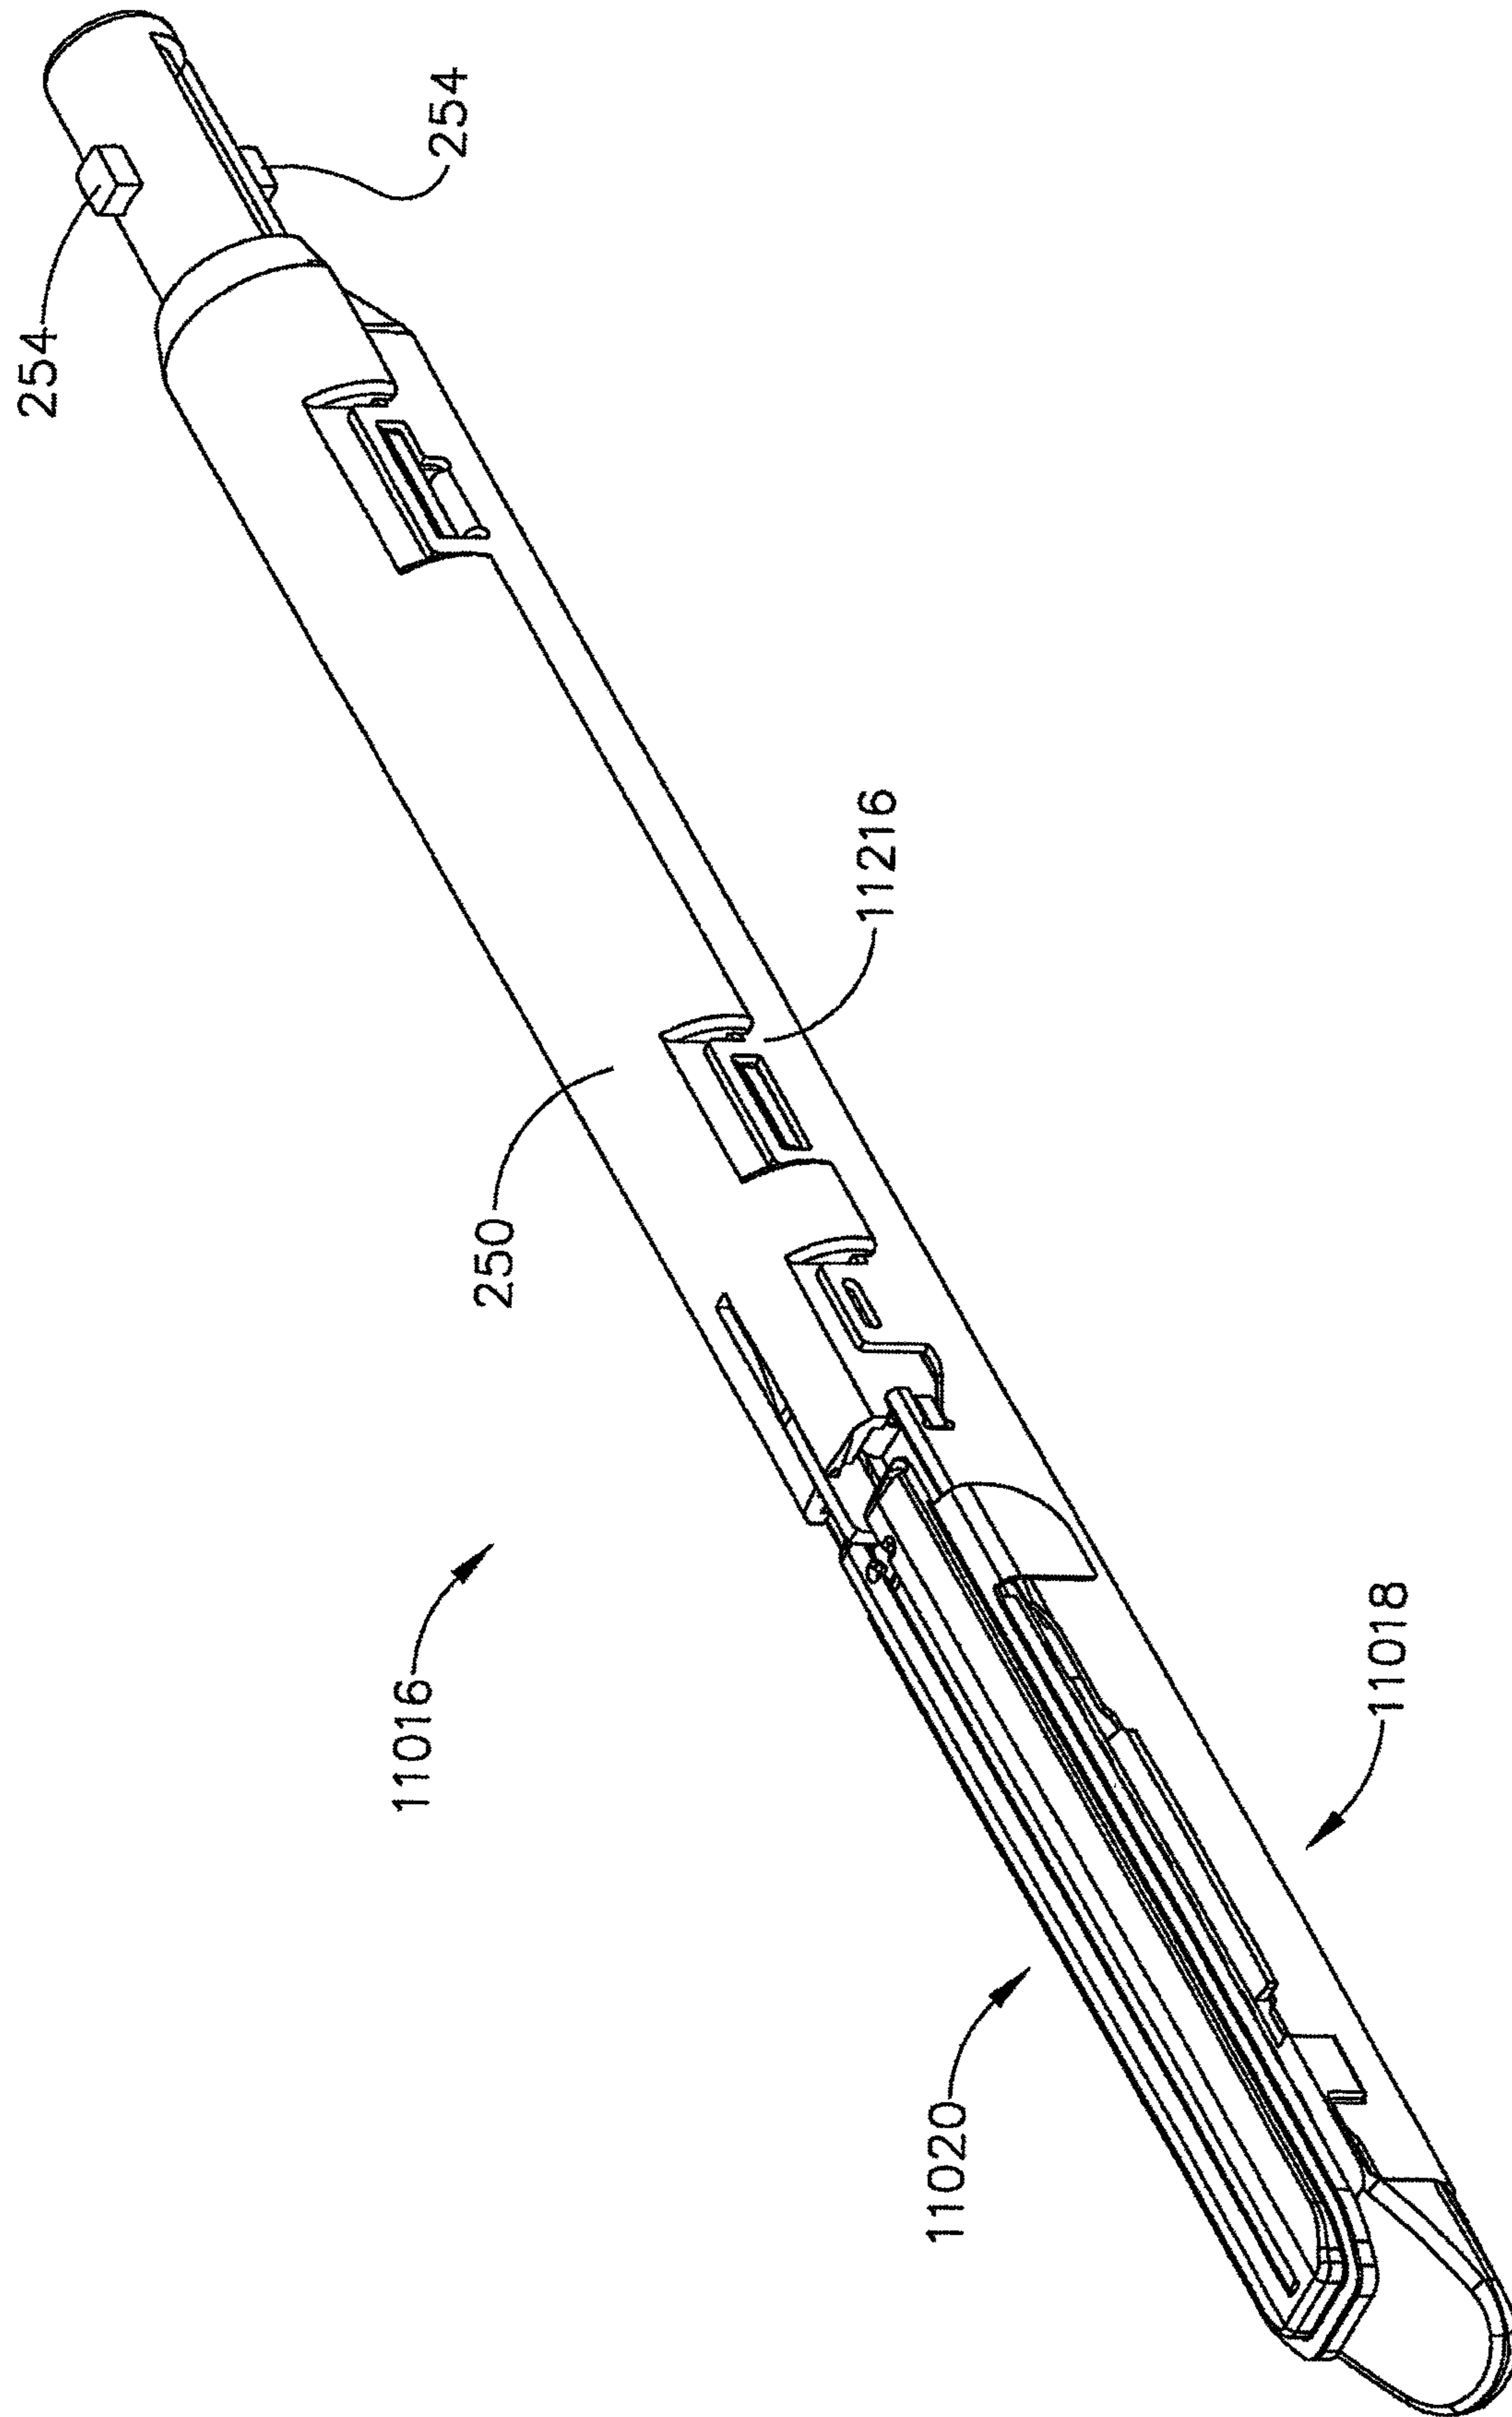


FIG. 131

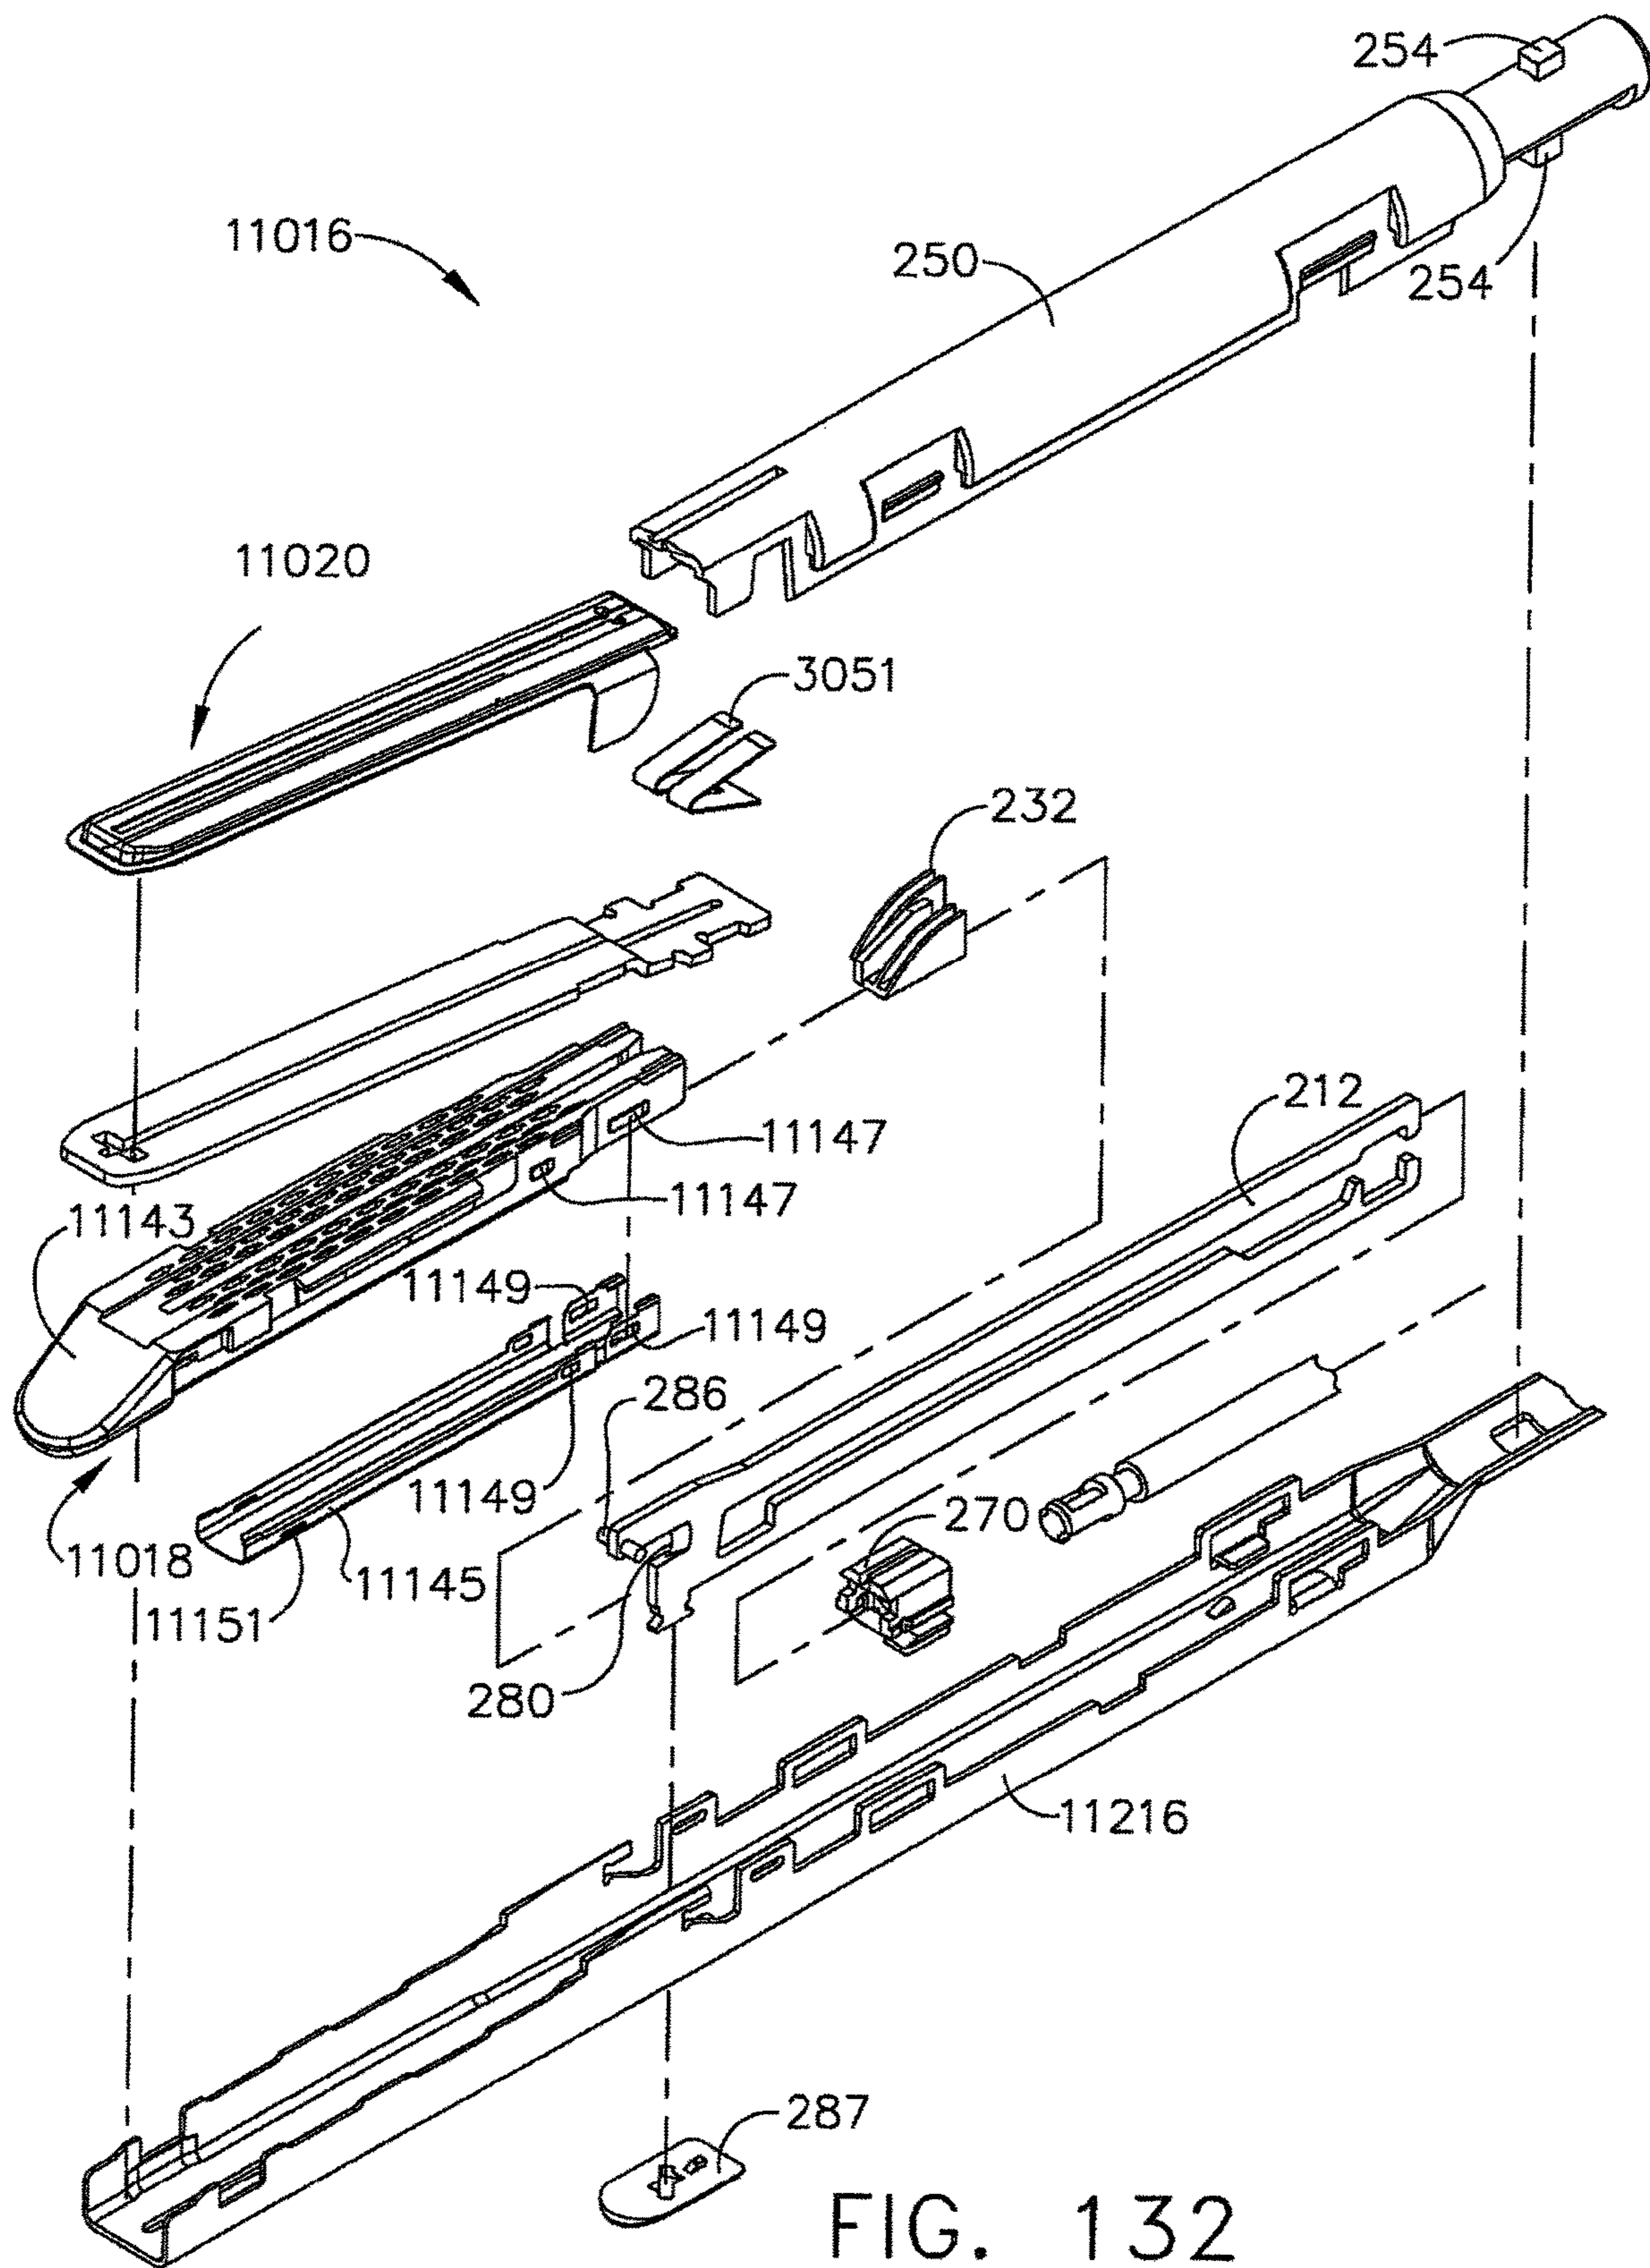


FIG. 132

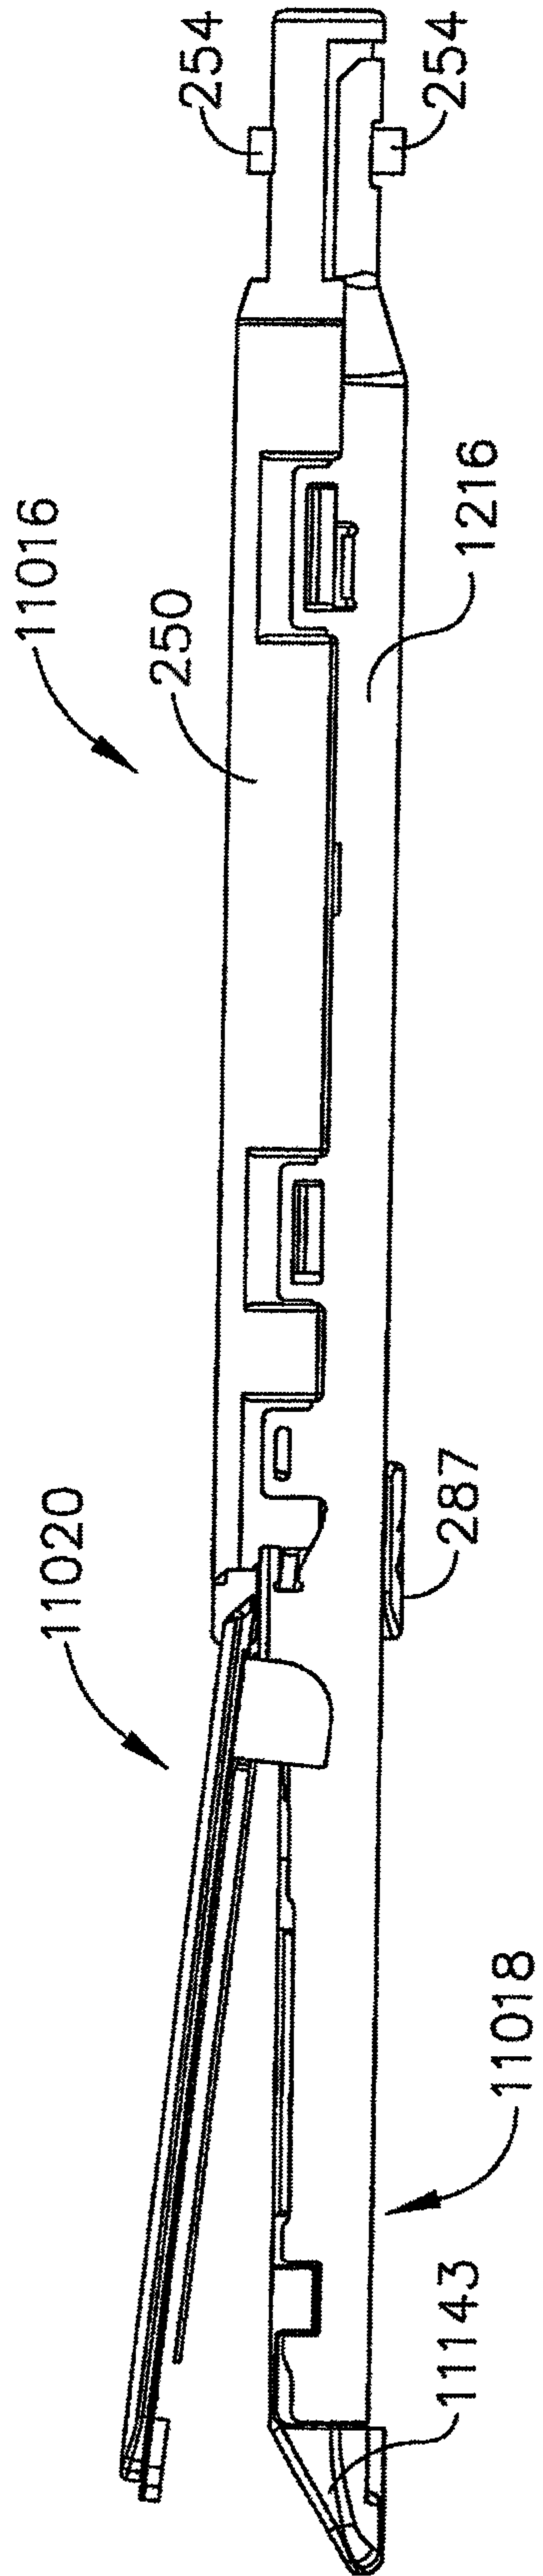


FIG. 133

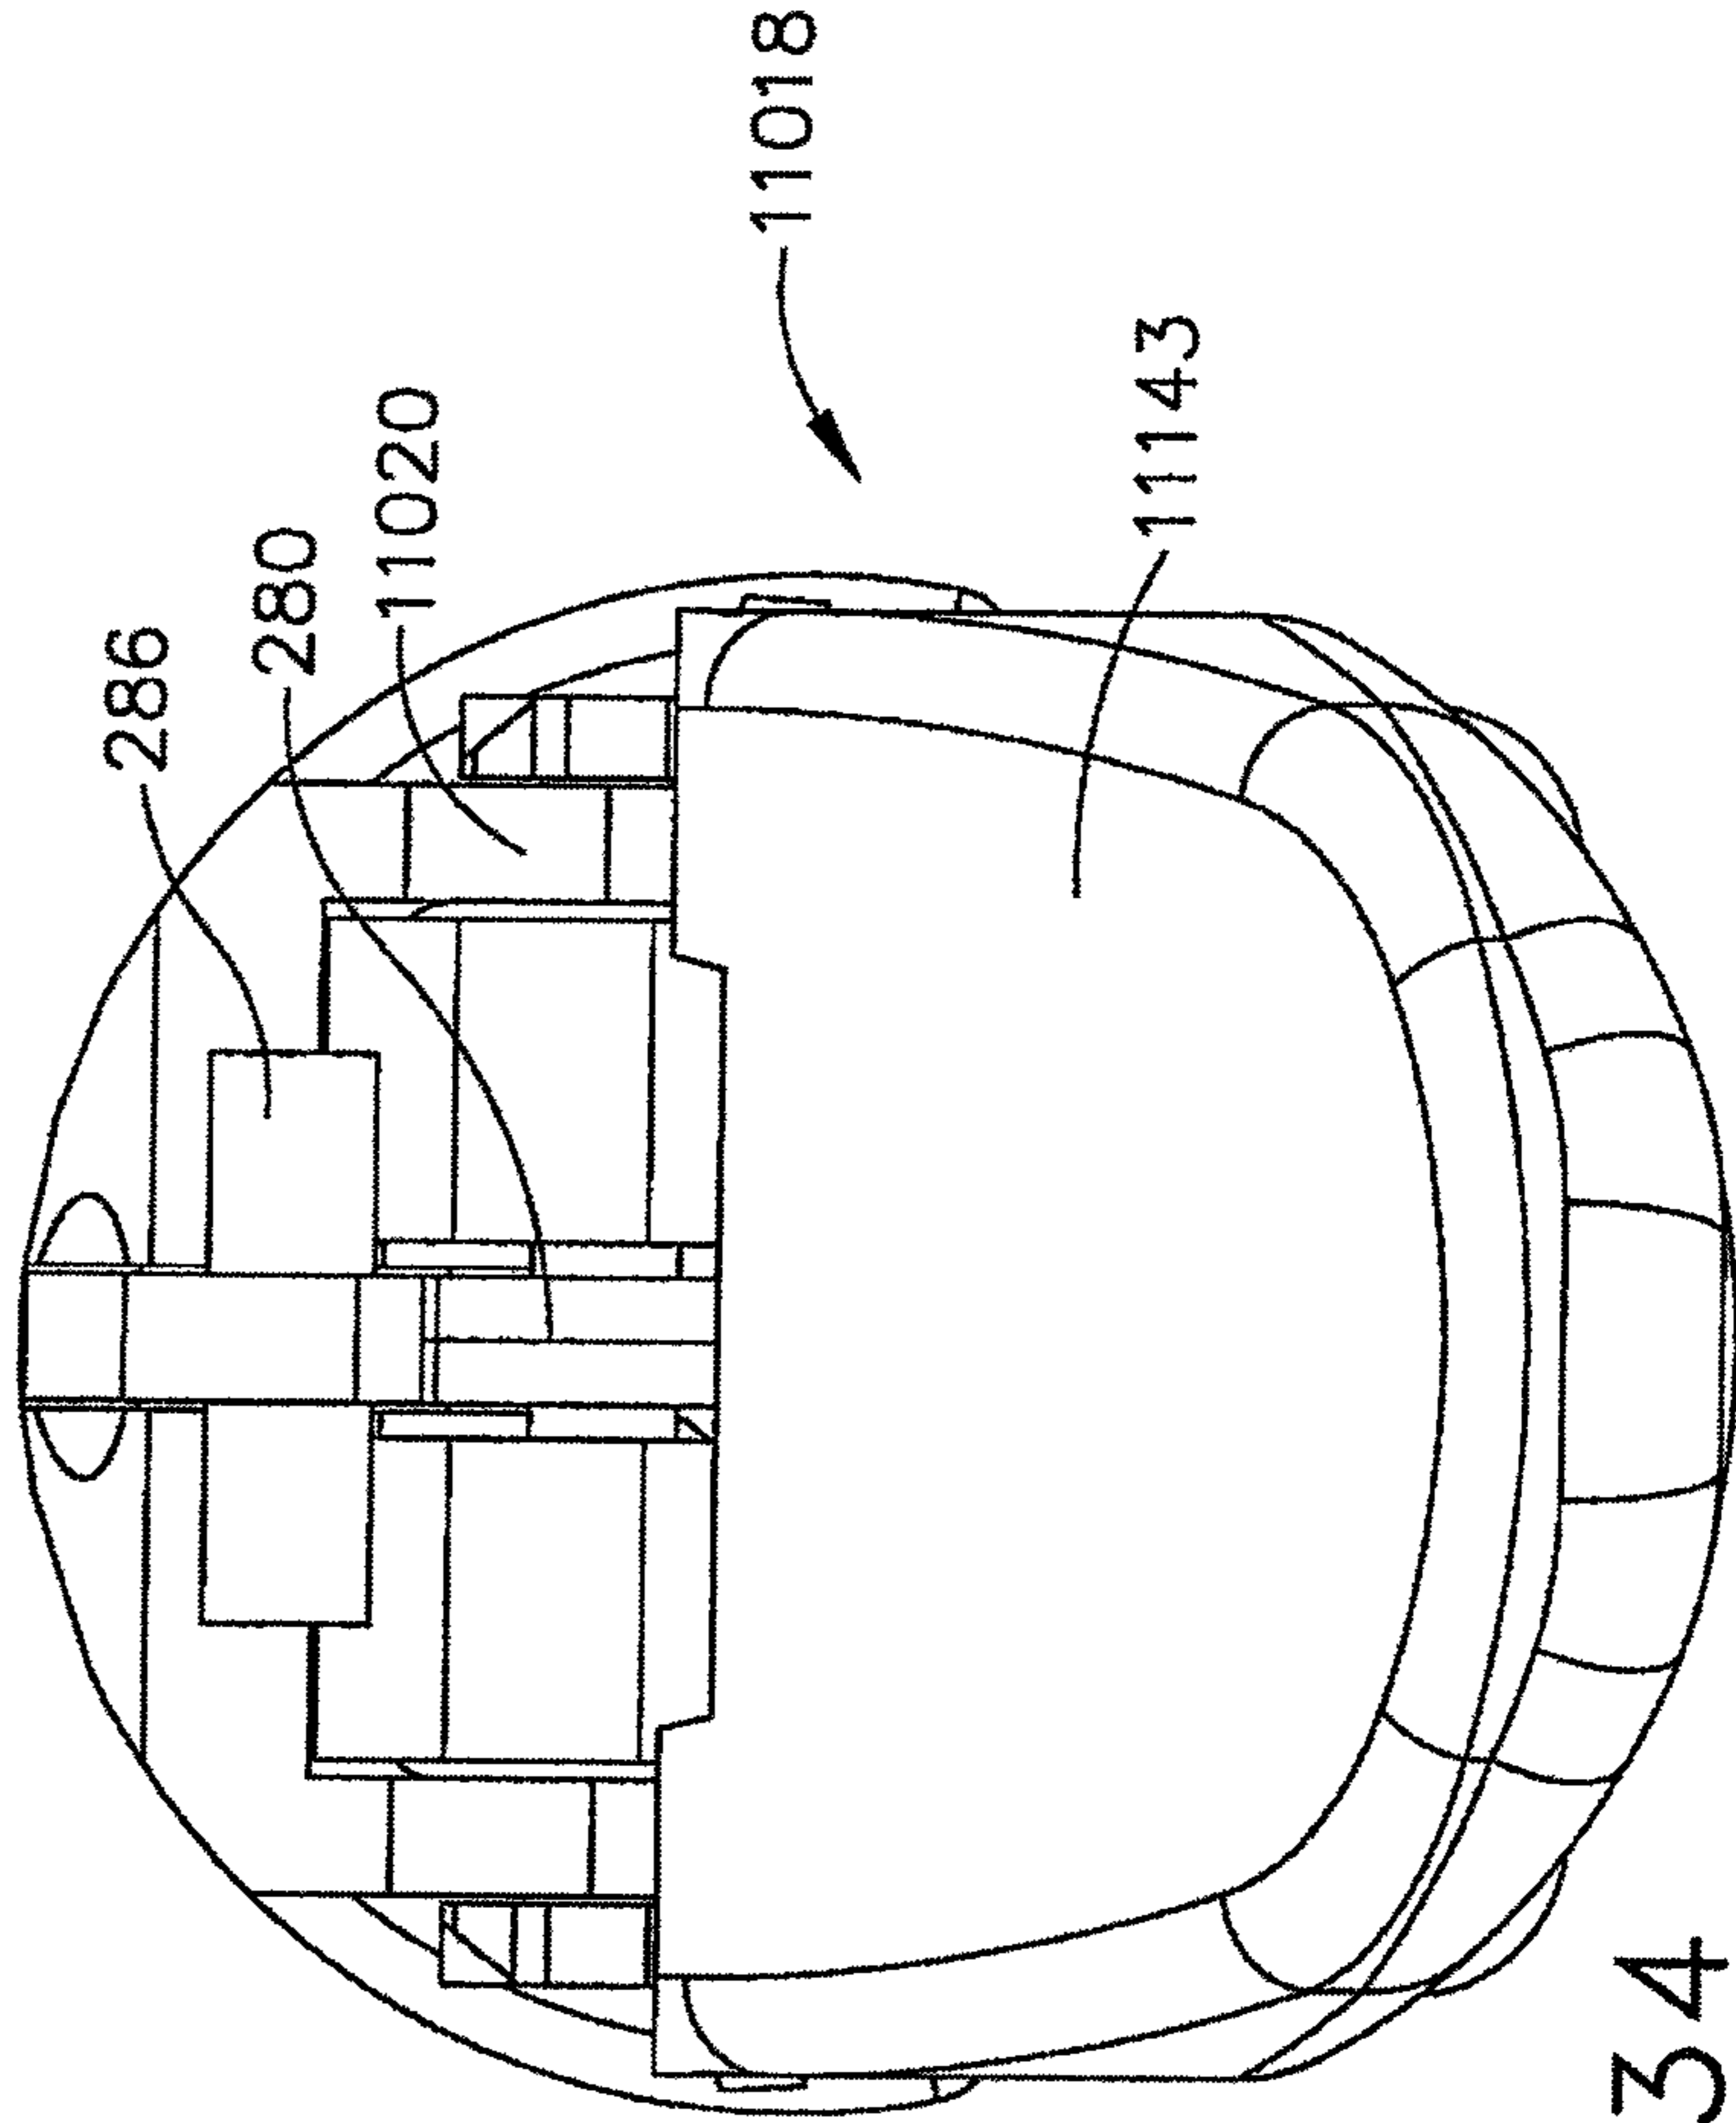


FIG. 134

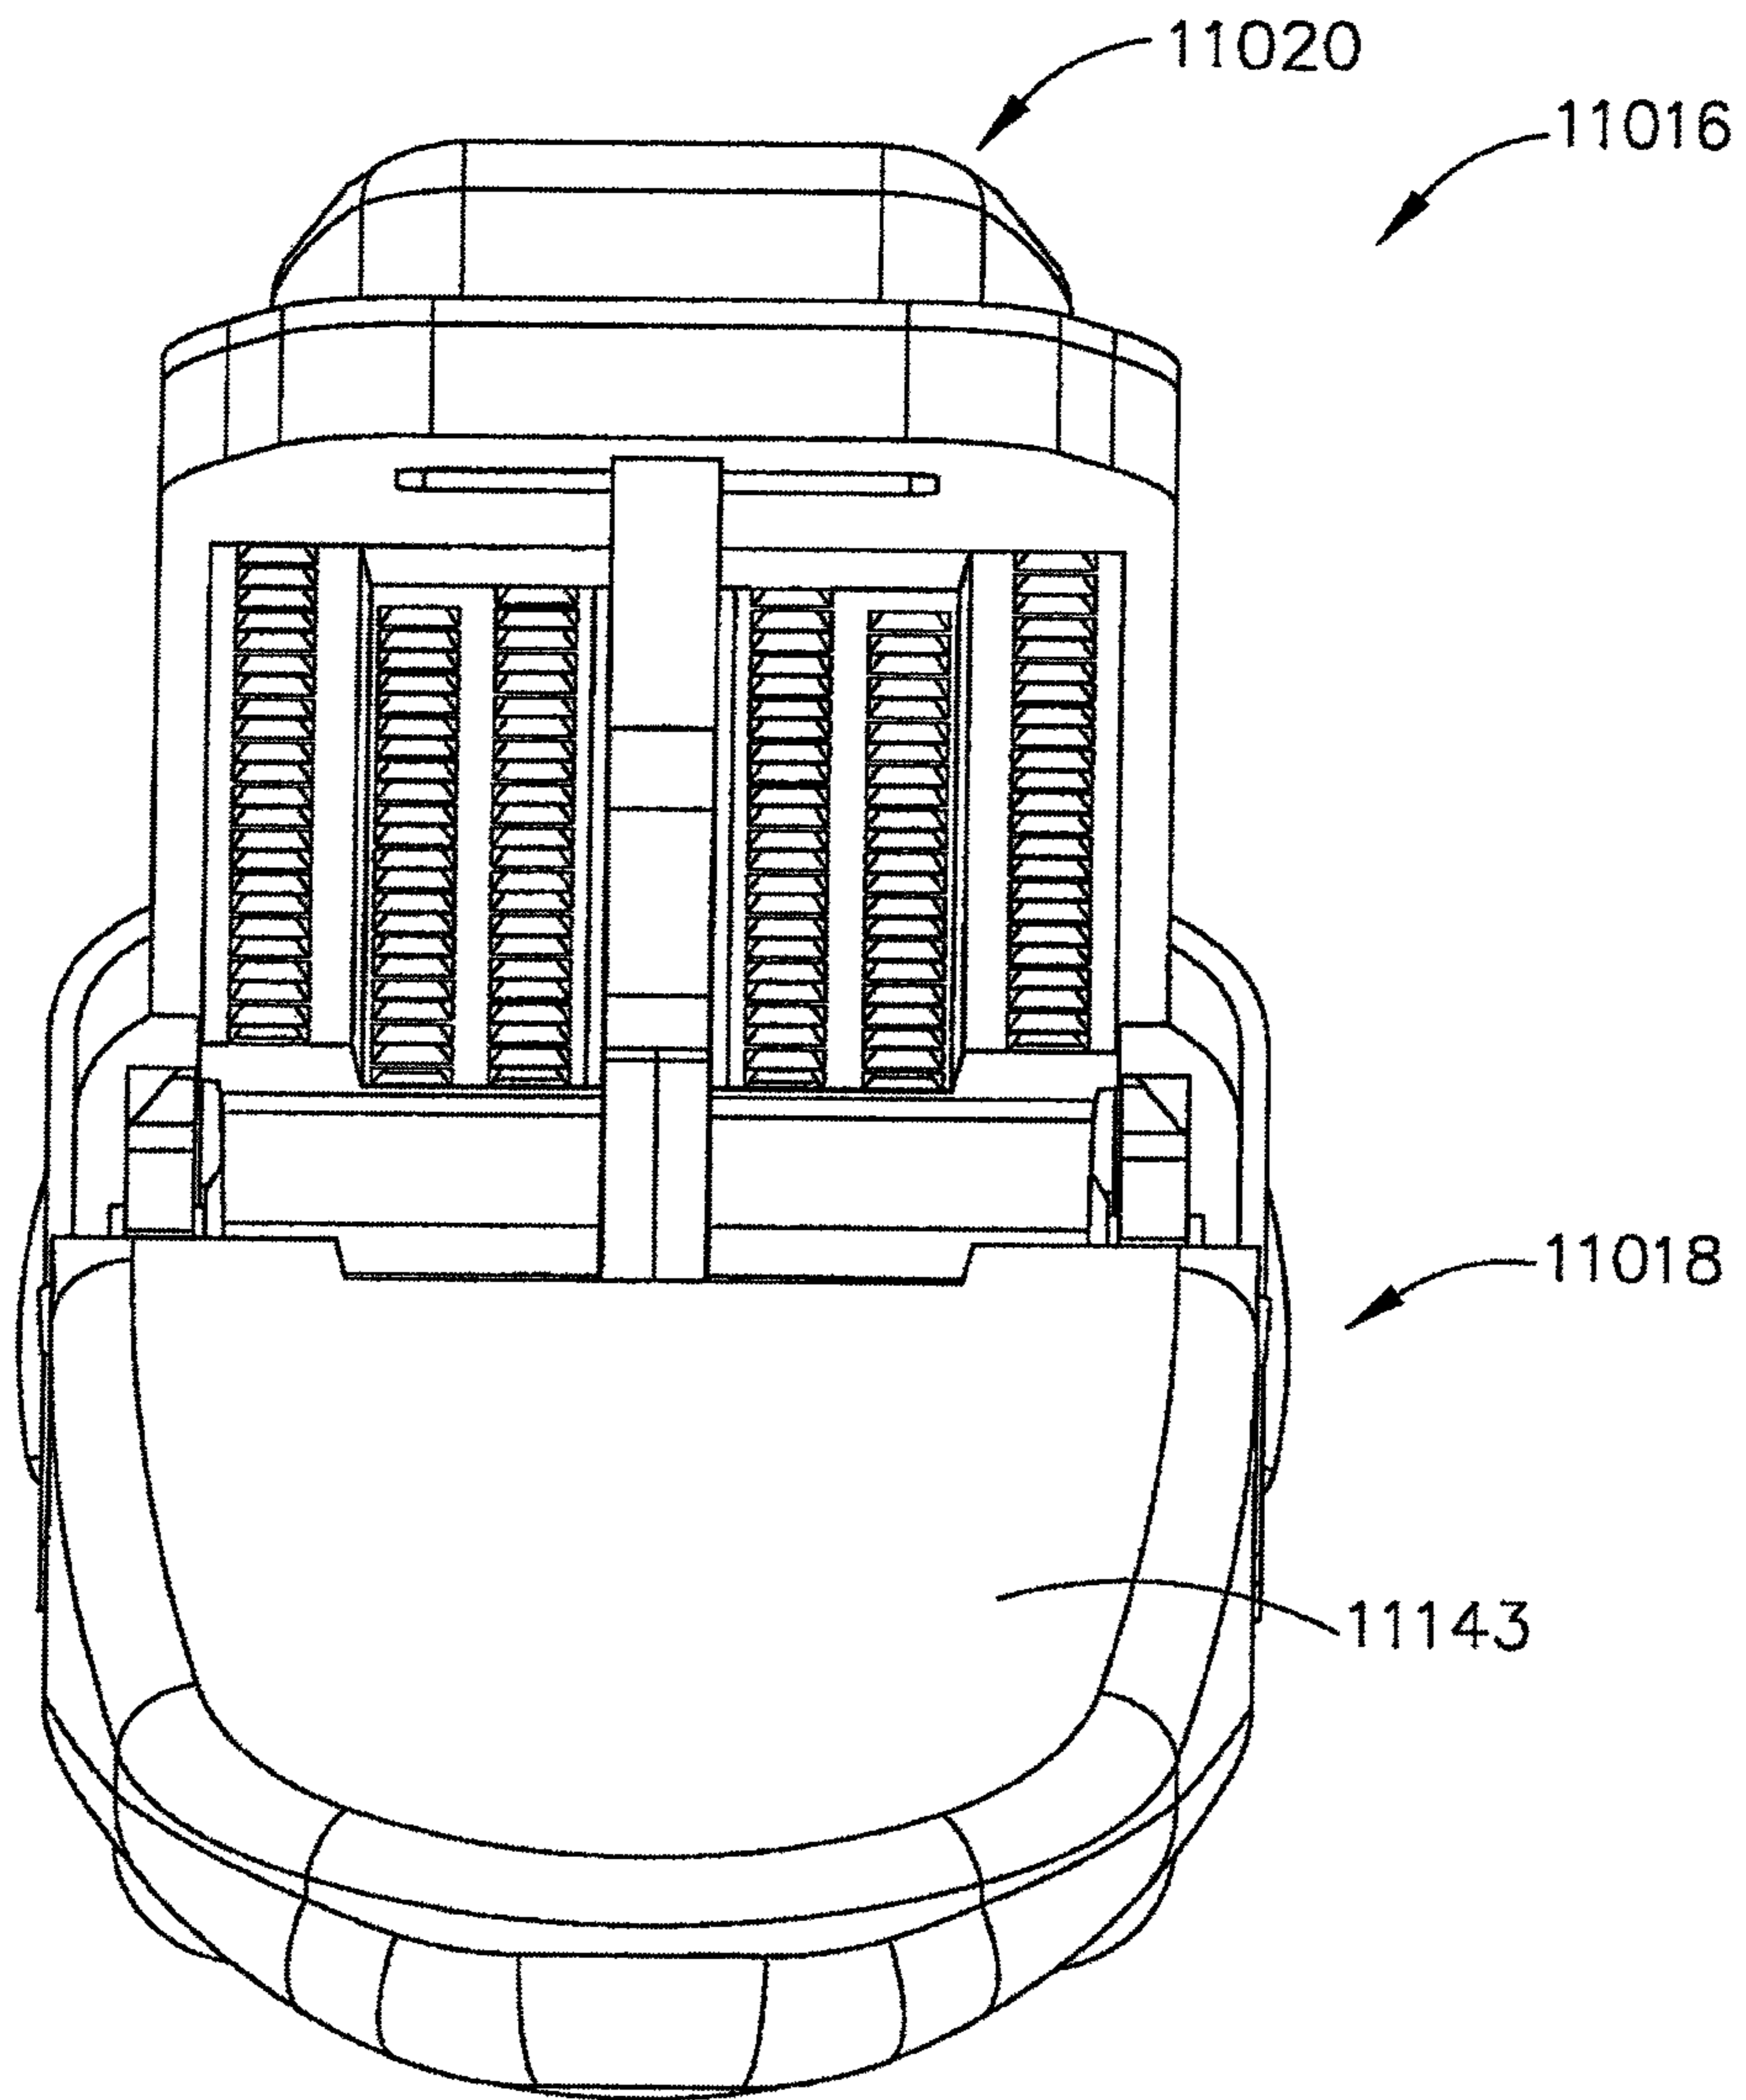


FIG. 135



**END EFFECTOR COUPLING  
ARRANGEMENTS FOR A SURGICAL  
CUTTING AND STAPLING INSTRUMENT**

CROSS-REFERENCE TO RELATED  
APPLICATIONS

This patent application is a continuation application claiming priority under 35 U.S.C. § 120 from Ser. No. 14/672,620, entitled DISPOSABLE LOADING UNIT FOR USE WITH A SURGICAL INSTRUMENT, filed Mar. 30, 2015, which issued on Mar. 13, 2018 as U.S. Pat. No. 9,913,647, which is a continuation application claiming priority under 35 U.S.C. § 120 from U.S. patent application Ser. No. 14/528,626, entitled END EFFECTOR COUPLING ARRANGEMENTS FOR A SURGICAL CUTTING AND STAPLING INSTRUMENT, filed Oct. 30, 2014, now U.S. Patent Application Publication No. 2015/0060521, which is a continuation application claiming priority under 35 U.S.C. § 120 from U.S. patent application Ser. No. 13/027,641, entitled END EFFECTOR COUPLING ARRANGEMENTS FOR A SURGICAL CUTTING AND STAPLING INSTRUMENT, filed Feb. 15, 2011, which issued on Nov. 4, 2014 as U.S. Pat. No. 8,875,972, which is a continuation application claiming priority under U.S.C. § 120 from U.S. patent application Ser. No. 12/031,817, entitled END EFFECTOR COUPLING ARRANGEMENTS FOR A SURGICAL CUTTING AND STAPLING INSTRUMENT, filed Feb. 15, 2008, now U.S. Patent Application Publication No. 2009/0206131, the entire disclosures of which are hereby incorporated by reference herein.

BACKGROUND

1. Technical Field

This application relates to a surgical stapling apparatus and, in various embodiments, to an articulating mechanism for use with an endoscopic surgical stapling apparatus for sequentially applying a plurality of surgical fasteners to body tissue and optionally incising fastened tissue.

2. Background of Related Art

Surgical devices wherein tissue is first grasped or clamped between opposing jaw structures and then joined by surgical fasteners are well known in the art. In some instruments, a knife is provided to cut the tissue which has been joined by the fasteners. The fasteners are typically in the form of surgical staples but two part polymeric fasteners can also be utilized.

Instruments for this purpose can include two elongated members which are respectively used to capture or clamp tissue. Typically, one of the members carries a staple cartridge which houses a plurality of staples arranged in at least two lateral rows while the other member has an anvil that defines a surface for forming the staple legs as the staples are driven from the staple cartridge. Generally, the stapling operation is effected by cam bars that travel longitudinally through the staple cartridge, with the cam bars acting upon staple pushers to sequentially eject the staples from the staple cartridge. A knife can travel between the staple rows to longitudinally cut and/or open the stapled tissue between the rows of staples. Such instruments are disclosed, for example, in U.S. Pat. Nos. 3,079,606 and 3,490,675, the entire disclosures of which are hereby incorporated by reference herein.

A later stapler disclosed in U.S. Pat. No. 3,499,591, the entire disclosure of which is hereby incorporated by reference herein, applies a double row of staples on each side of the incision. This is accomplished by providing a disposable loading unit in which a cam member moves through an elongate guide path between two sets of staggered staple carrying grooves. Staple drive members are located within the grooves and are positioned in such a manner so as to be contacted by the longitudinally moving cam member to effect ejection of the staples from the staple cartridge of the disposable loading unit. Other examples of such staplers are disclosed in U.S. Pat. Nos. 4,429,695 and 5,065,929, the entire disclosures of which are hereby incorporated by reference herein.

Each of the instruments described above were designed for use in conventional surgical procedures wherein surgeons have direct manual access to the operative site. However, in endoscopic or laparoscopic procedures, surgery is performed through a small incision or through a narrow cannula inserted through small entrance wounds in the skin. In order to address the specific needs of endoscopic and/or laparoscopic surgical procedures, endoscopic surgical stapling devices have been developed and are disclosed in, for example, U.S. Pat. Nos. 5,040,715; 5,307,976; 5,312,023; 5,318,221; 5,326,013; and 5,332,142, the entire disclosures of which are hereby incorporated by reference herein.

Many current laparoscopic linear stapling devices are configured to operate with disposable loading units and staple cartridges of only one size. For example, individual linear staplers are presently available for applying parallel rows of staples measuring 30 mm, 45 mm and 60 mm in length, for example. Thus, during a normal operation, a surgeon may be required to utilize several different stapling instruments to perform a single laparoscopic surgical procedure. Such practices increase the time, complexity and overall costs associated with laparoscopic surgical procedures. In addition, costs are greater in designing and manufacturing multiple stapler sizes, as opposed to creating a single, multipurpose stapler.

It would be extremely beneficial to provide a surgical device for use during laparoscopic and/or endoscopic surgical procedures that can be employed with several different sized disposable loading units to reduce the overall costs associated with such procedures. It would also be particularly beneficial if the device could perform multiple tasks, using disposable loading units of varying size and of varying purpose, such as, for example, to staple, clip, cut and/or articulate.

SUMMARY

In accordance with the present disclosure, improvements to a surgical stapling apparatus for sequentially applying a plurality of fasteners to body tissue and incising tissue are provided. In various embodiments, a surgical stapling apparatus includes a handle portion, an elongated body, or shaft, and a disposable loading unit, wherein the disposable loading unit is removably attachable to the elongated body. In at least one embodiment, the elongated body can include a connector portion which can be operably engaged with a connector portion of the disposable loading unit such that, when a trigger of the handle portion is actuated, the trigger can advance a driver within the disposable loading unit to deploy staples from the disposable loading unit and/or incise tissue. In previous surgical stapling devices, though, the disposable loading unit can become detached from the

elongate body causing the surgical stapling instrument to malfunction or be rendered inoperable.

In various embodiments of the present disclosure, such problems can be ameliorated by utilizing a surgical stapling instrument having a handle, a shaft extending from the handle, wherein the shaft defines an axis, and a disposable loading unit which is assembled to the shaft in a direction which is transverse to the shaft axis. Such a connection between the disposable loading unit and the shaft, in at least one embodiment, can prevent, or at least inhibit, the disposable loading unit from being unintentionally displaced proximally and/or distally relative to the shaft of the surgical instrument. In at least one embodiment, the surgical stapling instrument and/or disposable loading unit can further include a collar configured to threadably engage the shaft and/or a portion of the disposable loading unit. In various embodiments, a disposable loading unit and/or elongated body can include a detent assembly for holding the disposable loading unit in place after it has been assembled to the elongated body.

After a disposable loading unit has been attached to a surgical stapling instrument, the instrument can be positioned relative to the soft tissue of a patient. In various circumstances, a surgical stapling instrument can include an anvil and a staple cartridge, where the anvil can be rotated relative to the staple cartridge to position the anvil and the staple cartridge with respect to the soft tissue. In some surgical stapling instruments, the anvil can be configured to clamp the soft tissue between the anvil and the staple cartridge as staples are discharged from the staple cartridge. In various circumstances, a portion of the soft tissue can flow, or move, out of the distal end of the disposable loading unit and, as a result, the soft tissue may not be properly treated by the surgical stapling instrument.

In various embodiments of the present disclosure, such problems can be ameliorated by utilizing a surgical stapling instrument which can clamp the soft tissue, for example, prior to the staples being deployed from the staple cartridge. In various embodiments, a surgical stapling instrument can include an actuator configured to be retracted relative to the distal end of the disposable loading unit where the actuator can be operably engaged with the anvil to rotate the anvil between an open position and a closed position. In at least one embodiment, the actuator can include a cam, where the cam can include an arcuate profile having an apex, and where the apex can be configured to be in contact with the anvil when the anvil is in a closed position. In at least one such embodiment, the anvil can apply a clamping force to the soft tissue prior to the staples being deployed and prevent, or at least inhibit, the soft tissue from flowing, or 'milking', out of the distal end of the disposable loading unit.

In various embodiments of the present disclosure, a surgical stapling instrument can include a disposable loading unit comprising a staple cartridge, an anvil, and a sleeve, wherein the sleeve can be configured to be slid relative to the staple cartridge and the anvil. In at least one embodiment, the sleeve can include an aperture wherein the sleeve can be slid over at least a portion of the anvil and the staple cartridge to hold the anvil in a closed position. In at least one such embodiment, the sleeve can be slid into position to apply a clamping force to the soft tissue before staples are deployed into the soft tissue. In various embodiments, a surgical stapling instrument can include a tongue configured to be slid relative to a staple cartridge and an anvil, wherein the tongue can be configured to engage the anvil and hold the anvil in a closed position. In at least one embodiment, the

tongue can be configured such that it applies a force to the anvil at a distal end of the disposable loading unit so as to prevent, or at least reduce, soft tissue from milking out of the distal end.

After the anvil has been moved into a closed position, a drive beam can be advanced within the disposable loading unit to eject the staples therefrom and/or incise the soft tissue. In various circumstances, the anvil can include a slot defined therein which can be configured to receive at least a portion of the drive beam. In use, the drive beam can apply forces to the anvil which can cause the anvil to elastically and/or plastically deform and, as a result, affect the deployment of the surgical staples into the soft tissue. In various embodiments of the present disclosure, an anvil can include a first member having staple pockets for deforming the staples, a first cover plate secured to the first member, and a second cover plate secured to at least one of the first member and the first cover plate, wherein the first and second cover plates can be configured to support the first member. In at least one embodiment, an anvil can include a first member inserted into a second member, where the second member can be deformed such that the first member can be retained to and support the second member. In other various embodiments, the first member can be press-fit into the second member. In at least one embodiment, as a result of the above, the anvil can be better configured to withstand the forces applied thereto and eliminate, or at least reduce, undesirable deflections within the anvil.

In various circumstances, especially during endoscopic surgical procedures, at least a portion of a surgical stapling instrument is inserted through a cannula, or trocar, into a surgical site. Often, an anvil of a disposable loading unit is moved into its closed position before it is inserted into the trocar and then reopened after it has been inserted there-through. Some disposable loading units having large anvils and/or staple cartridges may not fit, or easily fit, through the trocar. In various embodiments of the present disclosure, a surgical stapling instrument can include a disposable loading unit having an anvil which can be moved between open, closed, and/or collapsed positions to facilitate the insertion of the disposable loading unit through the trocar. More particularly, in at least one embodiment, an anvil can be moved between a closed position in which the anvil is a first distance away from the staple cartridge, for example, and a collapsed position in which the anvil is closer to the staple cartridge such that the disposable loading unit can be more easily inserted through the trocar.

After the disposable loading unit has been used, or expended, it can be removed from the elongated body of the surgical instrument and a new disposable loading unit can be assembled to the elongated body. Thereafter, the surgical instrument can be reinserted into a surgical site to perform additional steps of a surgical technique. In various circumstances, though, a surgeon, or other clinician, may become confused as to whether a disposable loading unit has been previously expended. In various embodiments of the present disclosure, a disposable loading unit can include a lockout feature which can prevent, or at least inhibit, an expended disposable loading unit from being reassembled to the elongated body of the surgical instrument.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Various preferred embodiments are described herein with reference to the drawings:

FIG. 1 is a perspective view of one preferred embodiment of the presently disclosed surgical stapling apparatus;

## 5

FIG. 2 is a top view of the surgical apparatus shown in FIG. 1;

FIG. 3 is a side view of the surgical apparatus shown in FIG. 1;

FIG. 4 is a perspective view with parts separated of the handle assembly of the surgical apparatus shown in FIG. 1;

FIG. 5 is a cross-sectional view of a portion of the firing lockout mechanism shown in FIG. 4;

FIG. 6 is a perspective of the slide plate of the anti-reverse clutch mechanism of the surgical apparatus;

FIG. 7 is an enlarged perspective view of the anti-reverse clutch mechanism shown in FIG. 1;

FIG. 8 is a side cross-sectional view of the surgical stapling apparatus shown in FIG. 1 in the non-actuated position with the disposable loading unit removed;

FIG. 9 is a perspective view with parts separated of the rotation member, the articulation mechanism, and the elongated body of the surgical stapling apparatus shown in FIG. 1;

FIG. 10 is an enlarged view of the indicated area of detail shown in FIG. 8;

FIG. 10a is a perspective view of the translation member of the articulating mechanism and the proximal end of the elongated body of the surgical stapling apparatus shown in FIG. 1;

FIG. 10b is an enlarged cross-sectional view of the indicated area of detail of FIG. 8;

FIG. 10c is a cross-sectional view along section line 10c-10c of FIG. 8;

FIG. 11 is a perspective view of the cam member of the articulation mechanism of the surgical stapling apparatus shown in FIG. 1;

FIG. 12 is a top view of the cam member of the articulation mechanism of the surgical stapling apparatus shown in FIG. 1;

FIG. 12a is a perspective view of a non-articulating disposable loading unit usable with the surgical stapling apparatus shown in FIG. 1;

FIG. 12b is a perspective view of the preferred articulating disposable loading unit of the surgical stapling apparatus shown in FIG. 1;

FIG. 13 is a cross-sectional view taken along section line 13-13 of FIG. 10;

FIG. 14 is a cross-sectional view taken along section line 14-14 of FIG. 10;

FIG. 15 is a cross-sectional view taken along section line 15-15 of FIG. 10;

FIG. 16 is an enlarged view of the indicated area of detail shown in FIG. 8;

FIG. 17 is a side perspective view of the blocking plate of the surgical stapling apparatus shown in FIG. 1;

FIG. 18 is a top perspective view of the blocking plate of the surgical stapling apparatus shown in FIG. 1;

FIG. 19 is a perspective view of a disposable loading unit usable with the surgical stapling apparatus of FIG. 1;

FIG. 20 is another perspective view of a disposable loading unit usable with the surgical stapling apparatus of FIG. 1;

FIG. 21 is a perspective view of the tool assembly of the surgical stapling apparatus of FIG. 1 with parts separated;

FIG. 22 is an enlarged perspective view of the distal end of the anvil assembly showing a plurality of staple deforming cavities;

FIG. 23 is an enlarged perspective view of the distal end of the staple cartridge of the surgical stapling apparatus shown in FIG. 1;

## 6

FIG. 24 is a side cross-sectional view taken along section line 24-24 of FIG. 23;

FIG. 25 is a bottom perspective view of the staple cartridge shown in FIG. 21;

FIG. 26 is an enlarged perspective view of the actuation sled, the pushers and the fasteners shown in FIG. 21;

FIG. 27 is an enlarged perspective view with parts separated of the proximal housing portion and mounting assembly of the disposable loading unit shown in FIG. 19;

FIG. 28 is an enlarged perspective view of the mounting assembly of the disposable loading unit shown in FIG. 19 mounted to a distal end portion of the proximal housing portion;

FIG. 29 is an enlarged perspective view of the proximal housing portion and the mounting assembly of the disposable loading unit shown in FIG. 19 with the upper housing half removed;

FIG. 30 is a perspective view of the proximal housing portion and the mounting assembly of the disposable loading unit shown in FIG. 19 with the upper housing half removed;

FIG. 31 is a perspective view with parts separated of the axial drive assembly;

FIG. 32 is an enlarged perspective view of the axial drive assembly shown in FIG. 31;

FIG. 33 is an enlarged perspective view of the proximal end of the axial drive assembly shown in FIG. 31 including the locking device;

FIG. 34 is an enlarged perspective view of the distal end of the axial drive assembly shown in FIG. 31;

FIG. 35 is an enlarged perspective view of the distal end of the elongated body of the stapling apparatus shown in FIG. 1;

FIG. 36 is an enlarged perspective view of the locking device shown in FIG. 33;

FIG. 37 is an enlarged perspective view of a lower housing half of the proximal housing portion of the disposable loading unit shown in FIG. 27;

FIG. 38 is a side cross-sectional view of the disposable loading unit shown in FIG. 20;

FIG. 39 is an enlarged view of the indicated area of detail shown in FIG. 38;

FIG. 40 is a perspective view of the surgical stapling apparatus shown in FIG. 1 with the disposable loading unit of FIG. 19 detached from the elongated body;

FIG. 41 is an enlarged perspective view of the disposable loading unit of FIG. 19 during attachment to the elongated body of the surgical stapling apparatus shown in FIG. 1;

FIG. 42 is another enlarged perspective view of the disposable loading unit of FIG. 19 during attachment to the elongated body of the surgical stapling apparatus shown in FIG. 1;

FIG. 43 is a cross-sectional view taken along section line 43-43 of FIG. 41;

FIG. 43A is a side cross-sectional view of the rotation knob, articulation mechanism, and sensing mechanism during insertion of a disposable loading unit into the elongated body of the surgical stapling apparatus;

FIG. 44 is a cross-sectional view taken along section line 44-44 of FIG. 42;

FIG. 45 is a side cross-sectional view of the distal end of the disposable loading unit of FIG. 1 with tissue positioned between the anvil and clamp assemblies;

FIG. 46 is a side cross-sectional view of the handle assembly with the movable handle in an actuated position;

FIG. 47 is an enlarged view of the indicated area of detail shown in FIG. 46;

FIG. 48 is a cross-sectional view of the proximal end of the disposable loading unit of FIG. 19 and the distal end of the elongated body of the surgical stapling apparatus shown in FIG. 1 with the control rod in a partially advanced position;

FIG. 49 is a cross-sectional view of the tool assembly of the surgical stapling apparatus shown in FIG. 1 positioned about tissue in the clamped position;

FIG. 50 is a cross-sectional view of the handle assembly of the stapling apparatus of FIG. 1 during the clamping stroke of the apparatus;

FIG. 51 is a side cross-sectional view of the distal end of the tool assembly of the stapling apparatus shown in FIG. 1 during firing of the apparatus;

FIG. 52 is a side cross-sectional view of the distal end of the tool assembly of the stapling apparatus shown in FIG. 1 after firing of the apparatus;

FIG. 53 is a side cross-sectional view of the handle assembly of the apparatus during retraction of the actuation shaft;

FIG. 54 is a side cross-sectional view of the handle assembly of the stapling apparatus during actuation of the emergency release button;

FIG. 55 is a top view of the articulation mechanism of the surgical stapling apparatus;

FIG. 56 is a side cross-sectional view of the articulation mechanism and rotation member of the surgical stapling apparatus shown in FIG. 1;

FIG. 57 is a top view of the distal end of the elongated body, the mounting assembly, and the proximal end of the tool assembly during articulation of the stapling apparatus;

FIG. 58 is a perspective view of the surgical stapling apparatus during articulation of the tool assembly;

FIG. 59 is a perspective view of the surgical stapling apparatus during articulation and rotation of the tool assembly;

FIG. 60 is a top view of the distal end of the disposable loading unit immediately prior to articulation;

FIG. 61 is a top view of the distal end of the elongated body, the mounting assembly, and the proximal end of the tool assembly during articulation of the stapling apparatus;

FIG. 62 is a partial cross-sectional view of a portion of the disposable loading unit during retraction of the locking device;

FIG. 63 is a partial cross-sectional view of a portion of the disposable loading unit with the locking device in the locked position;

FIG. 64 is a partial perspective view of an elongated body and a disposable loading unit of an embodiment of a surgical stapling apparatus;

FIG. 65 is a perspective view of an embodiment of a surgical stapling apparatus including an elongated body defining an axis and a disposable loading unit;

FIG. 66 is a perspective view of a connector portion of the disposable loading unit of FIG. 65 and a connector portion of the elongated body of FIG. 65;

FIG. 67 is another perspective view of the connector portions of FIG. 66 with additional components of the disposable loading unit removed;

FIG. 68 is a cross-sectional perspective view of the connector portions of FIG. 66 assembled together and retained in position by a threaded collar;

FIG. 69 is a cross-sectional elevational view of the connector portions of FIG. 66 and the threaded collar of FIG. 68;

FIG. 70 is a cross-sectional view of a connector portion of a disposable loading unit assembled to a connector portion of an elongated body of an alternative embodiment of a surgical stapling apparatus;

FIG. 71 is a detail view of the connector portions of FIG. 70;

FIG. 72 is a cross-sectional view of the surgical stapling apparatus of FIG. 70 taken along line 72-72 in FIG. 71;

FIG. 73 is a detail view of an actuator of the elongated body of FIG. 70;

FIG. 74 is a perspective view of a disposable loading unit of an alternative embodiment of a surgical stapling apparatus;

FIG. 75 is an exploded view of the disposable loading unit of FIG. 74;

FIG. 76 is a cross-sectional view of the disposable loading unit of FIG. 74 including an anvil in an open position;

FIG. 76A is a detail view of the disposable loading unit of FIG. 74 illustrating an actuator operably engaged with the anvil;

FIG. 77 is a cross-sectional view of the disposable loading unit of FIG. 74 illustrating the anvil in a closed position;

FIG. 77A is a detail view of the anvil and actuator of the disposable loading unit of FIG. 76A;

FIG. 78 is a plan view of the disposable loading unit of FIG. 74 with some components removed;

FIG. 79 is a detail view of a portion of the disposable loading unit of FIG. 74;

FIG. 80 is a bottom plan view of the disposable loading unit of FIG. 74;

FIG. 81 is a cross-sectional view of a staple cartridge carrier of the disposable loading unit of FIG. 74;

FIG. 82 is a cross-sectional elevational view of an alternative embodiment of a disposable loading unit with some components removed, the disposable loading unit including an anvil in an open position;

FIG. 83 is a detail view of the disposable loading unit of FIG. 82 including an actuator for closing the anvil;

FIG. 84 is another cross-sectional elevational view of the disposable loading unit of FIG. 82 illustrating the anvil in a closed position;

FIG. 85 is a detail view of the actuator and the anvil of FIG. 83;

FIG. 86 is a perspective view of an anvil and an actuator of an alternative embodiment of a disposable loading unit;

FIG. 87 is a perspective view of an actuator of a further alternative embodiment of a disposable loading unit;

FIG. 88 is a perspective view of a drive beam of an alternative embodiment of a disposable loading unit;

FIG. 89 is an end view of the drive beam of FIG. 88;

FIG. 90 is a cross-sectional view of a portion of the drive beam of FIG. 88 positioned within a channel of an anvil;

FIG. 91 is a perspective view of a disposable loading unit of an alternative embodiment of a surgical stapling apparatus;

FIG. 92 is an end view of the disposable loading unit of FIG. 91;

FIG. 93 is a cross-sectional view of the disposable loading unit of FIG. 91;

FIG. 94 is a cross-sectional view of an alternative embodiment of a disposable loading unit;

FIG. 95 is a cross-sectional view of a further alternative embodiment of a disposable loading unit;

FIG. 96 is a cross-sectional view of another alternative embodiment of a disposable loading unit;

FIG. 97 is a cross-sectional view of an alternative embodiment of a disposable loading unit;

FIG. 98 is a perspective view of an anvil assembly of an alternative embodiment of a disposable loading unit, the anvil assembly including an outer portion and an insert portion;

FIG. 99 is a perspective view of the insert portion of FIG. 98;

FIG. 100 is a cross-sectional view of the insert positioned within the outer portion of the anvil assembly of FIG. 98;

FIG. 101 is a cross-sectional view of the anvil assembly of FIG. 98 illustrating the outer portion after it has been deformed to retain the insert portion therein;

FIG. 102 is a diagram of a piece of tubular stock having removed portions which are illustrated in dash;

FIG. 103 is a cross-sectional view of an anvil formed from the tubular stock of FIG. 102;

FIG. 104 is a cross-sectional view of an anvil assembly of an alternative embodiment of a disposable loading unit, the anvil assembly including an inner portion press-fit within an outer portion;

FIG. 105 is an end view of the inner portion of FIG. 104;

FIG. 106 is a cross-sectional view of an anvil assembly of an alternative embodiment of a disposable loading unit, the anvil assembly including a body and a support plate attached thereto;

FIG. 107 is a cross-sectional view of the anvil body of FIG. 106;

FIG. 108 is a cross-sectional view of the support plate of FIG. 106;

FIG. 109 is a perspective view of an alternative embodiment of a disposable loading unit including an anvil in a closed position and a sleeve in a retracted position;

FIG. 110 is a perspective view of the disposable loading unit of FIG. 109 illustrating the sleeve in an extended position to support the anvil;

FIG. 111 is a perspective view of an alternative embodiment of a disposable loading unit including an anvil in a closed position and a tongue in a retracted position;

FIG. 112 is a perspective view of the disposable loading unit of FIG. 111 illustrating the tongue in an extended position to support the anvil;

FIG. 113 is a cross-sectional view of the disposable loading unit of FIG. 111;

FIG. 114 is an exploded view of an alternative embodiment of a disposable loading unit;

FIG. 115 is a cross-sectional view of the disposable loading unit of FIG. 114 illustrating an anvil in an open position;

FIG. 116 is a detail view of the disposable loading unit of FIG. 114;

FIG. 117 is a cross-sectional view of the disposable loading unit of FIG. 114 illustrating the anvil in a closed position;

FIG. 118 is a detail view of the disposable loading unit of FIG. 116;

FIG. 119 is a cross-sectional view of the disposable loading unit of FIG. 114 illustrating the anvil in a collapsed position;

FIG. 120 is a detail view of the disposable loading unit of FIG. 114;

FIG. 121 is a cross-sectional view of the disposable loading unit of FIG. 114 illustrating the anvil in its collapsed position;

FIG. 122 is a cross-sectional view of the disposable loading unit of FIG. 114 illustrating the anvil returned to its closed position;

FIG. 123 is a perspective view of an alternative embodiment of a disposable loading unit;

FIG. 124 is a perspective view of a knife lockout of the disposable loading unit of FIG. 123;

FIG. 125 is a perspective view of the disposable loading unit of FIG. 123 with some components removed and a connector portion of an elongated body of a surgical stapling apparatus;

FIG. 126 is another perspective view of the disposable loading unit of FIG. 123;

FIG. 127 is another perspective view of the disposable loading unit of FIG. 123 with some components of the elongated body connector portion removed;

FIG. 128 is a perspective view of the disposable loading unit of FIG. 123 prior to a drive beam of the surgical apparatus being advanced within the disposable loading unit and a retention plate engaged with a biasing spring;

FIG. 129 is a perspective view of the disposable loading unit of FIG. 123 after the drive beam has been advanced the retention plate has been disengaged from the biasing spring;

FIG. 130 is a perspective view of the disposable loading unit of FIG. 123 after it has been disengaged from the connector portion of the elongated body illustrating the knife lockout biased into a locked-out position by the biasing spring;

FIG. 131 is a perspective view of an alternative embodiment of a disposable loading unit;

FIG. 132 is an exploded view of the disposable loading unit of FIG. 131 illustrating a removable staple cartridge;

FIG. 133 is an elevational view of the disposable loading unit of FIG. 131;

FIG. 134 is an end view of the disposable loading unit of FIG. 131; and

FIG. 135 is another end view of the disposable loading unit of FIG. 131 illustrating an anvil in an open position.

#### DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

Preferred embodiments of the presently disclosed endoscopic surgical stapling apparatus will now be described in detail with reference to the drawings, in which like reference numerals designate identical or corresponding elements in each of the several views. Those of ordinary skill in the art will understand that the devices and methods specifically described herein and illustrated in the accompanying drawings are non-limiting exemplary embodiments and that the scope of the various embodiments of the present invention is defined solely by the claims. The features illustrated or described in connection with one exemplary embodiment may be combined with the features of other embodiments. Such modifications and variations are intended to be included within the scope of the present invention.

In the drawings and in the description that follows, the term “proximal”, as is traditional, will refer to the end of the stapling apparatus which is closest to the operator, while the term distal will refer to the end of the apparatus which is furthest from the operator.

FIGS. 1-3 illustrate one embodiment of the presently disclosed surgical stapling apparatus shown generally as 10. Briefly, surgical stapling apparatus 10 includes a handle assembly 12 and an elongated body 14. A disposable loading unit or DLU 16 is releasably secured to a distal end of elongated body 14. Disposable loading unit 16 includes a tool assembly 17 having a cartridge assembly 18 housing a plurality of surgical staples and an anvil assembly 20 movably secured in relation to cartridge assembly 18. Disposable loading unit 16 is configured to apply linear rows of staples measuring from about 30 mm to about 60 mm in length.

## 11

Disposable loading units having linear rows of staples of other lengths are also envisioned, e.g., 45 mm. Handle assembly 12 includes a stationary handle member 22, a movable handle member 24, and a barrel portion 26. A rotatable member 28 is preferably mounted on the forward end of barrel portion 26 to facilitate rotation of elongated body 14 with respect to handle assembly 12. An articulation lever 30 is also preferably mounted on the forward end of barrel portion 26 adjacent rotatable knob 28 to facilitate articulation of tool assembly 17. A pair of retraction knobs 32 are movably positioned along barrel portion 26 to return surgical stapling apparatus 10 to a retracted position, as will be described in detail below.

Referring to FIG. 4, handle assembly 12 includes housing 36, which is preferably formed from molded housing half-sections 36a and 36b, which forms stationary handle member 22 and barrel portion 26 of handle assembly 12 (See FIG. 1). Movable handle member 24 is pivotably supported between housing half-sections 36a and 36b about pivot pin 38. A biasing member 40, which is preferably a torsion spring, biases movable handle 24 away from stationary handle 22. An actuation shaft 46 is supported within barrel portion 26 of housing 36 and includes a toothed rack 48. A driving pawl 42 having a rack engagement finger 43 with laterally extending wings 43a and 43b is pivotably mounted to one end of movable handle 24 about a pivot pin 44. A biasing member 50, which is also preferably a torsion spring, is positioned to urge engagement finger 43 of driving pawl 42 towards toothed rack 48 of actuation shaft 46. Movable handle 24 is pivotable to move engagement finger 43 of driving pawl 42 into contact with toothed rack 48 of actuation shaft 46 to advance the actuation shaft linearly in the distal direction. The forward end of actuation shaft 46 rotatably receives the proximal end 49 of a control rod 52 such that linear advancement of actuation shaft 46 causes corresponding linear advancement of control rod 52. A locking pawl 54 having a rack engagement member 55 is pivotably mounted within housing 36 about pivot pin 57 and is biased towards toothed rack 48 by biasing member 56, which is also preferably a torsion spring. Engagement member 55 of locking pawl 54 is movable into engagement with toothed rack 48 to retain actuation shaft 46 in a longitudinally fixed position.

A retraction mechanism 58 which includes a pair of retractor knobs 32 (See FIG. 1) is connected to the proximal end of actuation shaft 46 by a coupling rod 60. Coupling rod 60 includes right and left engagement portions 62a and 62b for receiving retractor knobs 32 and a central portion 62c which is dimensioned and configured to translate within a pair of longitudinal slots 34a formed in actuation shaft 46 adjacent the proximal end thereof. A release plate 64 is operatively associated with actuation shaft 46 and is mounted for movement with respect thereto in response to manipulation of retractor knobs 32. A pair of spaced apart pins 66 extend outwardly from a lateral face of actuation shaft 46 to engage a pair of corresponding angled cam slots 68 formed in release plate 64. Upon rearward movement of retractor knobs 32, pins 66 can release plate 64 downwardly with respect to actuation shaft 46 and with respect to toothed rack 48 such that the bottom portion of release plate 64 extends below toothed rack 48 to disengage engagement finger 43 of driving pawl 42 from toothed rack 48. A transverse slot 70 is formed at the proximal end of release plate 64 to accommodate the central portion 62c of coupling rod 60, and elongated slots 34 (See FIG. 1) are defined in the barrel section 26 of handle assembly 12 to accommodate the longitudinal translation of coupling rod 60 as retraction

## 12

knobs 32 are pulled rearwardly to retract actuation shaft 46 and thus retract control rod 52 rearwardly. Actuation shaft 46 is biased proximally by spring 72 which is secured at one end to coupling rod portion 62 via connector 74 and at the other end to post 76 on actuation shaft 46.

Referring also to FIG. 5, handle assembly 12 includes a firing lockout assembly 80 which includes a plunger 82 and a pivotable locking member 83. Plunger 82 is biased to a central position by biasing springs 84 and includes annular tapered camming surfaces 85. Each end of plunger 82 extends through housing 36 (See FIG. 1) adjacent an upper end of stationary handle 22. Pivotable locking member 83 is pivotably attached at its distal end between housing half-sections 36a and 36b about pivot pin 86 and includes a locking surface 88 and proximal extension 90 having a slot 89 formed therein. Locking member 83 is biased by spring 92 counter-clockwise (as viewed in FIG. 4) to move locking surface 88 to a position to abut the distal end of actuation shaft 46 to prevent advancement of shaft 46 and subsequent firing of stapling apparatus 10. Annular tapered camming surface 85 is positioned to extend into tapered slot 89 in proximal extension 90. Lateral movement of plunger 82 in either direction against the bias of either spring 84 moves tapered camming surface 85 into engagement with the sidewalls of tapered slot 89 to pivot locking member 83 clockwise about pivot pin 86, as viewed in FIG. 4, to move blocking surface 88 to a position to permit advancement of actuation shaft 46 and thus firing of stapling apparatus 10. Blocking surface 88 is retained in this position by recesses 87 which receive the tapered tip of camming surface 85 to lock locking member 83 in a counter-clockwise position. Operation of firing lockout assembly 80 will be further illustrated below.

Referring to FIGS. 4, 6, and 7, handle mechanism 12 also includes an anti-reverse clutch mechanism which includes a first gear 94 rotatably mounted on a first shaft 96, and second gear 98 mounted on a second shaft 100, and a slide plate 102 (FIGS. 6 and 7) slidably mounted within housing 36. Slide plate 102 includes an elongated slot 104 dimensioned and configured to be slidably positioned about locking pawl pivot pin 57, a gear plate 106 configured to mesh with the teeth of second gear 98, and a cam surface 108. In the retracted position, cam surface 108 of slide plate 102 engages locking pawl 54 to prevent locking pawl 54 from engaging toothed rack 48. Actuation shaft 46 includes a distal set of gear teeth 110a spaced from a proximal set of gear teeth 110b positioned to engage first gear 94 of actuation shaft 46 during movement of actuation shaft 46. When actuation shaft 46 is advanced by pivoting movable handle 24 about pivot pin 38, distal gear teeth 110a on actuation shaft 46 mesh with and rotate first gear 94 and first shaft 96. First shaft 96 is connected to second shaft 100 by spring clutch assembly such that rotation of first shaft 96 will cause corresponding rotation of second shaft 100. Rotation of second shaft 100 causes corresponding rotation of second gear 98 which is engaged with gear plate 106 on slide plate 102 to cause linear advancement of slide plate 102. Linear advancement of slide plate 102 is limited to the length of elongated slot 104. When slide plate has been advanced the length of slot 104, cam surface 108 releases locking pawl 54 such that it is moved into engagement with toothed rack 48. Continued advancement of actuation shaft 46 eventually moves gear teeth 110b into engagement with gear plate 106. However, since slide plate 102 is longitudinally fixed in position, the spring clutch is forced to release, such that continued distal advancement of actuation shaft 46 is permitted.

## 13

When actuation shaft **46** is returned to the retracted position (by pulling retraction knobs **34** proximally, as discussed above) gear teeth **110b** engage first gear **94** to rotate second gear **98** in the reverse direction to retract slide member **102** proximally within housing **36**. Proximal movement of slide member **102** advances cam surface **108** into locking pawl **54** prior to engagement between locking pawl **54** and toothed rack **48** to urge locking pawl **54** to a position to permit retraction of actuation shaft **46**.

Referring again to FIG. 4, handle assembly **12** includes an emergency return button **112** pivotally mounted within housing **36** about a pivot member **114** supported between housing half-sections **36a** and **36b**. Return button **112** includes an externally positioned member **116** positioned on the proximal end of barrel portion **26**. Member **116** is movable about pivot member **114** into engagement with the proximal end of locking pawl **54** to urge rack engagement member **55** out of engagement with toothed rack **48** to permit retraction of actuation shaft **46** during the firing stroke of the stapling apparatus **10**. As discussed above, during the clamping portion of advancement of actuation shaft **46**, slide plate **102** disengages pawl **54** from rack **48** and thus actuation of return button **112** is not necessary to retract the actuation shaft **46**.

FIG. 8 illustrates the interconnection of elongated body **14** and handle assembly **12**. Referring to FIGS. 8-10, housing **36** includes an annular channel **117** configured to receive an annular rib **118** formed on the proximal end of rotation member **28**, which is preferably formed from molded half-sections **28a** and **28b**. Annular channel **117** and rib **118** permit relative rotation between rotation member **28** and housing **36**. Elongated body **14** includes inner housing **122** and an outer casing **124**. Inner housing **122** is dimensioned to be received within outer casing **124** and includes an internal bore **126** (FIG. 8) which extends therethrough and is dimensioned to slidably receive a first articulation link **123** and control rod **52**. The proximal end of housing **122** and casing **124** each include a pair of diametrically opposed openings **130** and **128**, respectively, which are dimensioned to receive radial projections **132** formed on the distal end of rotation member **28**. Projections **132** and openings **128** and **130** fixedly secure rotation member **28** and elongated body **14** in relation to each other, both longitudinally and rotatably. Rotation of rotation knob **28** with respect to handle assembly **12** thus results in corresponding rotation of elongated body **14** with respect to handle assembly **12**.

An articulation mechanism **120** is supported on rotatable member **28** and includes articulation lever **30**, a cam member **136**, a translation member **138**, and first articulation link **123** (FIG. 9). Articulation lever **30** is pivotally mounted about pivot member **140** which extends outwardly from rotation member **28** and is preferably formed integrally therewith. A projection **142** extends downwardly from articulation lever **30** for engagement with cam member **136**.

Referring temporarily to FIGS. 11 and 12, cam member **136** includes a housing **144** having an elongated slot **146** extending through one side thereof and a stepped camming surface **148** formed in the other side thereof. Each step of camming surface **148** corresponds to a particular degree of articulation of stapling apparatus **10**. Although five steps are illustrated, fewer or more steps may be provided. Elongated slot **146** is configured to receive projection **142** formed on articulation lever **30**. Housing **144** includes a distal stepped portion **150** and a proximal stepped portion **152**. Proximal stepped portion **152** includes a recess **154**.

Referring again to FIGS. 8-10 and also to FIGS. 13-15, translation member **138** includes a plurality of ridges **156** which are configured to be slidably received within grooves

## 14

**158** formed along the inner walls of rotation member **28**. Engagement between ridges **156** and grooves **158** prevent relative rotation of rotation member **28** and translation member **138** while permitting relative linear movement. The distal end of translation member **138** includes arm **160** which includes an opening **162** configured to receive a finger **164** extending from the proximal end of articulation link **123** (See FIG. 10a). A pin **166** having a housing **168** constructed from a non-abrasive material, e.g., Teflon, is secured to translation member **138** and dimensioned to be received within stepped camming surface **148**.

In an assembled condition, proximal and distal stepped portions **150** and **152** of cam member **136** are positioned beneath flanges **170** and **172** formed on rotation member **28** to restrict cam member **136** to transverse movement with respect to the longitudinal axis of stapling apparatus **10**. When articulation lever **30** is pivoted about pivot member **140**, cam member **136** is moved transversely on rotation member **28** to move stepped camming surface **148** transversely relative to pin **166**, forcing pin **166** to move proximally or distally along stepped cam surface **148**. Since pin **166** is fixedly attached to translation member **138**, translation member **138** is moved proximally or distally to effect corresponding proximal or distal movement of first articulation link **123**.

Referring to FIGS. 8-10 and 16, a disposable loading unit sensing mechanism extends within stapling apparatus **10** from elongated body **14** into handle assembly **12**. The sensing mechanism includes a sensor tube **176** which is slidably supported within bore **26** of elongated body **14**. The distal end of sensor tube **176** is positioned towards the distal end of elongated body **14** and the proximal end of sensor tube **176** is secured within the distal end of a sensor cylinder **178** via a pair of nubs **180**. The distal end of a sensor link **182** is secured to the proximal end of sensor cylinder **178**. Sensor link **182** (See FIGS. 8a and 8c) has a bulbous end **184** which engages a camming surface **83a** on pivotable locking member **83**. When a disposable loading unit (not shown) is inserted in the distal end of elongated body **14**, the disposable loading unit engages the distal end **177** of sensor tube **176** to drive sensor tube **176** proximally, and thereby drive sensor cylinder **178** and sensor link **182** proximally. Movement of sensor link **182** proximally causes bulbous end **184** of sensor link **182** to move distally of camming surface **83a** to allow locking member **83** to pivot under the bias of spring **92** from a position permitting firing of stapling apparatus **10** to a blocking position, wherein blocking member **83** is positioned to engage actuation shaft **46** and prevent firing of stapling apparatus **10**. Sensor link **182** and locking member **83** function to prevent firing of surgical stapling apparatus **10** after a disposable loading unit has been secured to elongated body **14**, without first operating firing lockout assembly **80**. It is noted that movement of link **182** proximally permits locking member **83** to move to its position shown in FIG. 5.

Referring again to FIGS. 9-12, cam member **136** includes recess **154**. A locking ring **184** having a nub portion **186** configured to be received within recess **154** is positioned about sensor cylinder **178** between a control tab portion **188** and a proximal flange portion **190**. A spring **192** positioned between flange portion **190** and locking ring **184** urges locking ring distally about sensor cylinder **178**. When an articulating disposable loading unit **16b** having an extended insertion tip **193** is inserted into the distal end of elongated body **14** of stapling apparatus **10**, insertion tip **193** causes tab portion **188** to move proximally into engagement with locking ring **184** to urge locking ring **184** and nub **186**

proximally of recess 154 in cam member 136 (See FIG. 12b). With nub 186 positioned proximally of recess 154, cam member 136 is free to move transversely to effect articulation of stapling apparatus 10. A non-articulating disposable loading unit does not have an extended insertion tip (See FIG. 12a). As such, when a non-articulating disposable loading unit is inserted in elongated body 14, sensor cylinder 178 is not retracted proximally a sufficient distance to move nub 186 from recess 154. Thus, cam member 136 is prevented from moving transversely by nub 186 of locking ring 184 which is positioned in recess 154 and articulation lever 30 is locked in its central position.

Referring to FIGS. 16-18, the distal end of elongated body 14 includes a control rod locking mechanism 190 which is activated during insertion of a disposable loading unit into elongated body 14. Control rod locking mechanism 190 includes a blocking plate 192 which is biased distally by a spring 194 and includes a proximal finger 189 having angled cam surface 195. A semi-circular engagement member 196 is biased transversely towards control rod 52 by a spring 197. Control rod 52 includes an annular recess 199 configured to receive engagement member 196. Blocking plate 192 is movable from a distal position spaced from engagement member 196 to a proximal position located behind engagement member 196. In the proximal position, engagement member 196 is prevented from being biased from recess 199 by engagement with blocking plate 192. During insertion of a disposable loading unit 16 (See FIG. 1) into the distal end of elongated body 14, as will be described in further detail below, cam surface 195 of blocking plate 192 is engaged by a nub 254 (FIG. 30) on the disposable loading unit 16 as the disposable loading unit is rotated into engagement with elongated body 14 to urge plate 192 to the proximal position. Engagement member 196, which is positioned within recess 199, is retained therein by blocking plate 192 while nub 254 engages cam surface 195 to prevent longitudinal movement of control rod 52 during assembly. When the disposable loading unit 16 is properly positioned with respect to the elongated body 14, nub 254 on the proximal end of the disposable loading unit 16 passes off cam surface 195 allowing spring 194 to return blocking plate 192 to its distal position to permit subsequent longitudinal movement of control rod 52. It is noted that when the disposable loading unit nub passes off cam surface 195, an audible clicking sound is produced indicating that the disposable loading unit 16 is properly fastened to the elongated body 14.

Referring to FIGS. 19 and 20, disposable loading unit 16 includes a proximal housing portion 200 adapted to releasably engage the distal end of body portion 14 (FIG. 1). A mounting assembly 202 is pivotally secured to the distal end of housing portion 200, and is configured to receive the proximal end of tool assembly 17 such that pivotal movement of mounting assembly 202 about an axis perpendicular to the longitudinal axis of housing portion 200 effects articulation of tool assembly 17.

Referring to FIGS. 21-26, tool assembly 17 preferably includes anvil assembly 20 and cartridge assembly 18. Anvil assembly 20 includes anvil portion 204 having a plurality of staple deforming concavities 206 (FIG. 22) and a cover plate 208 secured to a top surface of anvil portion 204 to define a cavity 210 (FIG. 24) therebetween. Cover plate 208 is provided to prevent pinching of tissue during clamping and firing of stapling apparatus 10. Cavity 210 is dimensioned to receive a distal end of an axial drive assembly 212 (See FIG. 27). A longitudinal slot 214 extends through anvil portion 204 to facilitate passage of retention flange 284 of axial

drive assembly 212 into the anvil cavity 210. A camming surface 209 formed on anvil portion 204 is positioned to engage axial drive assembly 212 to facilitate clamping of tissue 198. A pair of pivot members 211 formed on anvil portion 204 are positioned within slots 213 formed in carrier 216 to guide the anvil portion between the open and clamped positions. A pair of stabilizing members 215 engage a respective shoulder 217 formed on carrier 216 to prevent anvil portion 204 from sliding axially relative to staple cartridge 220 as camming surface 209 is deformed.

Cartridge assembly 18 includes a carrier 216 which defines an elongated support channel 218. Elongated support channel 218 is dimensioned and configured to receive a staple cartridge 220. Corresponding tabs 222 and slots 224 formed along staple cartridge 220 and elongated support channel 218 function to retain staple cartridge 220 within support channel 218. A pair of support struts 223 formed on staple cartridge 220 are positioned to rest on side walls of carrier 216 to further stabilize staple cartridge 220 within support channel 218.

Staple cartridge 220 includes retention slots 225 for receiving a plurality of fasteners 226 and pushers 228. A plurality of spaced apart longitudinal slots 230 extend through staple cartridge 220 to accommodate upstanding cam wedges 232 of actuation sled 234. A central longitudinal slot 282 extends along the length of staple cartridge 220 to facilitate passage of a knife blade 280. During operation of surgical stapler 10, actuation sled 234 translates through longitudinal slots 230 of staple cartridge 220 to advance cam wedges 232 into sequential contact with pushers 228, to cause pushers 228 to translate vertically within slots 224 and urge fasteners 226 from slots 224 into the staple deforming cavities 206 of anvil assembly 20.

Referring to FIGS. 27 and 28, mounting assembly 202 includes upper and lower mounting portions 236 and 238. Each mounting portion includes a threaded bore 240 on each side thereof dimensioned to receive threaded bolts 242 (See FIG. 21) for securing the proximal end of carrier 216 thereto. A pair of centrally located pivot members 244 (See FIG. 21) extends between upper and lower mounting portions via a pair of coupling members 246 which engage the distal end of housing portion 200. Coupling members 246 each include an interlocking proximal portion 248 configured to be received in grooves 250 formed in the proximal end of housing portion 200 to retain mounting assembly 202 and housing portion 200 in a longitudinally fixed position in relation thereto.

Housing portion 200 of disposable loading unit 16 includes an upper housing half 250 and a lower housing half 252 contained within an outer casing 251. The proximal end of housing half 250 includes engagement nubs 254 for releasably engaging elongated body 14 and an insertion tip 193. Nubs 254 form a bayonet type coupling with the distal end of body 14 which will be discussed in further detail below. Housing halves 250 and 252 define a channel 253 for slidably receiving axial drive assembly 212. A second articulation link 256 is dimensioned to be slidably positioned within a slot 258 formed between housing halves 250 and 252. A pair of blow out plates 254 are positioned adjacent the distal end of housing portion 200 adjacent the distal end of axial drive assembly 212 to prevent outward bulging of drive assembly 212 during articulation of tool assembly 17.

Referring to FIGS. 29-30, second articulation link 256 includes at least one elongated metallic plate. Preferably, two or more metallic plates are stacked to form link 256. The proximal end of articulation link 256 includes a hook portion 258 configured to engage first articulation link 123 (See FIG.



9) and the distal end includes a loop 260 dimensioned to engage a projection 262 formed on mounting assembly 202. Projection 262 is laterally offset from pivot pin 244 such that linear movement of second articulation link 256 causes mounting assembly 202 to pivot about pivot pins 244 to articulate tool assembly 17.

Referring also to FIGS. 31-34, axial drive assembly 212 includes an elongated drive beam 266 including a distal working head 268 and a proximal engagement section 270. Drive beam 266 may be constructed from a single sheet of material or, preferably, multiple stacked sheets. Engagement section 270 includes a pair of engagement fingers 270a and 270b which are dimensioned and configured to mountingly engage a pair of corresponding retention slots 272a and 272b formed in drive member 272. Drive member 272 includes a proximal porthole 274 configured to receive the distal end 276 of control rod 52 (See FIG. 35) when the proximal end of disposable loading unit 16 is engaged with elongated body 14 of surgical stapling apparatus 10.

The distal end of drive beam 266 is defined by a vertical support strut 278 which supports a knife blade 280, and an abutment surface 283 which engages the central portion of actuation sled 234 during a stapling procedure. Surface 285 at the base of surface 283 is configured to receive a support member 287 slidably positioned along the bottom of the staple cartridge 220. Knife blade 280 is positioned to translate slightly behind actuation sled 234 through a central longitudinal slot 282 in staple cartridge 220 (FIG. 30) to form an incision between rows of stapled body tissue. A retention flange 284 projects distally from vertical strut 278 and supports a cylindrical cam roller 286 at its distal end. Cam roller 286 is dimensioned and configured to engage cam surface 209 on anvil body 204 to clamp anvil portion 204 against body tissue.

Referring also to FIGS. 36-39, a locking device 288 is pivotally secured to drive member 270 about a pivot pin 290. Locking device 288 includes a pair of elongate glides 292 and 294 which define a channel 296. A web 298 joins a portion of the upper surfaces of glides 292 and 294, and is configured and dimensioned to fit within elongated slot 298 formed in drive beam 266 at a position distal of drive member 270. Horizontal cams 300 and 302 extend from glides 292 and 294 respectively, and are accommodated along an inner surface of lower housing half 252. As best shown in FIG. 42, a torsion spring 304 is positioned adjacent drive member 270 and engages horizontal cams 300 and 302 of locking device 288 to normally bias locking device 288 downward toward lower housing half 252 onto ledge 310. Locking device 288 translates through housing portion 200 with axial drive assembly 212. Operation of locking device 288 will be described below.

#### Sequence of Operation

Referring to FIGS. 40-44, to use stapling instrument 10, a disposable loading unit 16 is first secured to the distal end of elongated body 14. As discussed above, stapling instrument 10 can be used with articulating and non-articulating disposable loading units having linear rows of staples between about 30 mm and about 60 mm. To secure disposable loading unit 16 to elongated body 14, the distal end 276 of control rod 52 is inserted into insertion tip 193 of disposable loading unit 16, and insertion tip 193 is slid longitudinally into the distal end of elongated body 14 in the direction indicated by arrow "A" in FIG. 41 such that hook portion 258 of second articulation link 256 slides within a channel 310 in elongated body 314. Nubs 254 will each be aligned in a respective channel (not shown) in elongated body 14. When hook portion 258 engages the proximal wall

312 of channel 310, disposable loading unit 16 is rotated in the direction indicated by arrow "B" in FIGS. 41-44 to move hook portion 258 of second articulation link 256 into engagement with finger 164 of first articulation link 123. Nubs 254 also forms a bayonet type coupling within annular channel 314 in body 14. During rotation of loading unit 16, nubs 254 engage cam surface 195 (FIG. 41) of block plate 192 to initially move plate 192 in the direction indicated by arrow "C" in FIGS. 41 and 43 to lock engagement member 196 in recess 199 of control rod 52 to prevent longitudinal movement of control rod 52 during attachment of disposable loading unit 16. During the final degree of rotation, nubs 254 disengage from cam surface 195 to allow blocking plate 192 to move in the direction indicated by arrow "D" in FIGS. 42 and 44 from behind engagement member 196 to once again permit longitudinal movement of control rod 52.

Referring to FIGS. 43 and 43a, when insertion tip 193 engages the distal end of sensor tube 176, the disposable loading unit sensing mechanism is actuated. Insertion tip 193 engages and moves sensor tube 176 proximally in the direction indicated by arrow "E" in FIG. 43. As discussed above, proximal movement of sensor tube 176 effects proximal movement of sensor cylinder 178 and sensor link 182 in the direction indicated by arrow "E" in FIG. 43a to pivot locking member 83 counter-clockwise, as indicated by arrow "Y" in FIG. 43a, from a non-blocking position to a position blocking movement of actuation shaft 46.

Referring to FIGS. 46-49, with a disposable loading unit attached to stapling instrument 10, tool assembly 17 can be positioned about tissue 320 (FIG. 45). To clamp tissue between anvil assembly 20 and cartridge assembly 18, stationary handle 24 is moved in the direction indicated by arrow "E" in FIG. 46 against the bias of torsion spring 40 to move driving pawl 42 into engagement with shoulder 322 on actuation shaft 46. Engagement between shoulder 322 and driving pawl 42 advances actuation shaft 46 and thus advances control rod 52 distally. Control rod 52 is connected at its distal end to axial drive assembly 212 (FIG. 48), including drive beam 266, such that distal movement of control rod 52 effects distal movement of drive beam 266 in the direction indicated by arrow "F" in FIGS. 48 and 49, moving cam roller 286 into engagement with cam surface 209 on anvil portion 204 to urge anvil portion 204 in the direction indicated by arrow "G" in FIG. 49. It is noted that one complete stroke of movable handle 24 advances actuation shaft 46 approximately 15 mm which is sufficient to clamp tissue during the first stroke but not to fire staples.

As discussed above with respect to the anti-reverse clutch mechanism, during the first (clamping) stroke of movable handle 24, slide plate 102 (FIG. 46) prevents locking pawl 54 from engaging toothed rack 48. To maintain actuation shaft 46 in its longitudinal position after handle 24 is released, an engagement member 324 (FIG. 47) is provided on locking member 83 to engage shoulder 326 on actuation shaft 46 and retain shaft 46 in its longitudinal position (See FIG. 47). Upon release of movable handle 24, drive pawl 42 moves over rack 48 as torsion spring 40 returns handle 24 to a position spaced from stationary handle 22. In this position, driving pawl 42 is urged into engagement with toothed rack 48 to retain actuation shaft 46 in its longitudinal fixed position.

In order to fire staples, movable handle 24 is actuated again, i.e., moved through another stroke. As discussed above, stapling apparatus 10 is capable of receiving disposable loading units having linear rows of staples of between about 30 mm and about 60 mm. Since each stroke of the movable handle 24 preferably advances actuation shaft 46

15 mm, and one stroke is required to clamp tissue, the movable handle must be actuated (n+1) strokes to fire staples, where n is the length of the linear rows of staples in the disposable loading unit attached to stapling instrument 10 divided by 15 mm.

Referring to FIG. 50, prior to being able to fire staples, firing lockout assembly 80 (FIG. 4) must be actuated to move locking surface 88 from its blocking position (FIG. 47) to a non-blocking position. This is accomplished by pressing down on plunger 82 to move camming surface 85 into engagement with sidewalls of slot 89 of locking member 83 to pivot locking member 83 in the direction indicated by arrow "G" in FIG. 50 (see also FIG. 5). Thereafter, movable handle 24 may be actuated an appropriate number of strokes to advance actuation shaft 46, and thus control rod 52 and drive beam 266, distally in the direction indicated by arrow "H" in FIGS. 51 and 52 to advance actuation sled 234 through staple cartridge 220 to effect ejection of staples. It is noted that after the first or clamping stroke of movable handle 54 (during the second stroke), slide 102 passes over locking pawl 54 allowing torsion spring 56 to move locking pawl 54 in the direction indicated by arrow "I" in FIG. 50 into engagement with toothed rack 48 to retain actuation shaft 46 in its longitudinal position.

Referring to FIG. 53, to retract actuation shaft 46 and thus control rod 52 and drive member 266 after firing staples, retraction knobs 32 (see FIG. 1) are pulled proximally causing pins 66 to move release plate 64 in the direction indicated by arrow "J" in FIG. 53 over teeth 48 to disengage drive pawl 42 from engagement with teeth 48. As discussed above, with respect to the anti-reverse clutch mechanism, locking pawl 54 is urged by slide plate 102 out of engagement with toothed rack 48 (not shown) to permit actuation shaft 46 to be moved proximally, in the direction indicated by arrow "L", after drive pawl 42 is disengaged from teeth 48.

Referring to FIG. 54, in order to retract actuation shaft 46 prior to firing stapling apparatus, i.e., when locking pawl is currently engaged with toothed rack 48, emergency return button 112 is pushed in the direction indicated by arrow "Z" in FIG. 54 to disengage locking pawl 54 from toothed rack 48. Retraction knobs 32 (FIG. 1) must also be concurrently pulled rearwardly, as discussed above, to release drive pawl 42 from rack 48.

Referring to FIGS. 55-61, when an articulating disposable loading unit is secured to elongated body 14 and articulation lever 30 is pivoted in the direction indicated by arrow "M" in FIG. 55, cam member 136 is moved transversely by projection 142 (FIG. 10) in the direction indicated by arrow "N" between flanges 170 and 172 of rotation knob 28. Since translation member 138 is prevented from rotating by ridges 156 (FIG. 13), pin 166, which is fixedly secured to translation member 138, is forced to move along stepped cam surface 148. Movement of pin 166 causes corresponding movement of translation member 138 in the direction indicated by arrow "P" in FIGS. 55 and 56 to advance first articulation link 123 in the distal direction. The distal end of first articulation link 123 engages the proximal end of second articulation link 256 (FIG. 42) which is connected to projection 262 on mounting assembly 202 to advance second link 256 in the direction indicated by arrow "Q" in FIG. 57. Projection 262 is laterally offset from pivot members 244, such that distal advancement of second articulation link 256 causes mounting assembly 202 and thus tool assembly 17 to pivot in the direction indicated by arrow "R" in FIGS. 57 and 58. Note in FIG. 59 that rotation member 28 can be

rotated to rotate elongated body 14 about its longitudinal axis while tool assembly 17 is articulated.

FIGS. 60-61 illustrate articulation of tool assembly 17 in the opposite direction to that described above. When second articulation link 256 is retracted by rotating articulation lever 30 in a counter-clockwise direction (not shown) as viewed in FIG. 55, pin 66 is forced to move proximally along stepped camming surface 148, moving translation member 138 and first articulation link 123 proximally. Movement of first articulation link 123 proximally, causes second articulation link 256 to move proximally as indicated by arrow "S" in FIG. 58, to rotate tool assembly 17 in a clockwise direction, as indicated by arrow "T" in FIG. 61.

Referring to FIG. 12, movement of pin 166 (FIG. 9) between adjacent step portions 340 causes tool assembly 17 to articulate 22.5 degrees. Camming surface 148 includes five step portions 340. The third step portion corresponds to the non-articulated tool assembly position, whereas the first and the fifth step portions correspond to articulation of tool assembly 17 to forty-five degrees. Each step portion is flat to retain articulation lever 30 in a fixed position when pin 166 is engaged therewith.

Referring now to FIGS. 37, 39, 62 and 63, the sequence of lockout operation will be described in detail. In FIG. 39, lockout device 288 is shown in its prefired position with horizontal cams 300 and 302 resting on top of projections 330 formed in the sidewalls of lower housing half 252 (FIG. 37). In this position, locking device 288 is held up out of alignment with projection 332 formed in the bottom surface of lower housing half 252, and web 298 is in longitudinal juxtaposition with shelf 334 defined in drive beam 266. This configuration permits the anvil 20 (FIG. 38) to be opened and repositioned onto the tissue to be stapled until the surgeon is satisfied with the position without activating locking device 288 to disable the disposable loading unit 16.

As shown in FIG. 62, upon distal movement of drive beam 266, locking device 288 rides off of projections 330 (not shown) and is biased into engagement with base lower housing half 252 by spring 304, distal to projection 332. Locking device 288 remains in this configuration throughout firing of the apparatus.

Upon retraction of the drive beam 266 in the direction indicated by arrow "U" in FIG. 62, locking device 288 passes under projections 330 and rides over projection 332 until the distalmost portion of locking device 288 is proximal to projection 332. Spring 304 biases locking device 288 into juxtaposed alignment with projection 332, effectively disabling the disposable loading unit. If an attempt is made to reactuate the apparatus, the control rod 52 will abut a proximal end surface of locking device 288 which surface is diagonally sloped to impart a moment about pivot pin 342 such that the distal end of locking device 288 is rotationally urged into contact with projection 332. Continued distal force in the direction indicated by arrow "W" in FIG. 63, will only serve to increase the moment applied to the locking device thus the locking device will abut projection 332 and inhibit distal movement of the control rod 52.

Referring again to FIGS. 41-44, the disabled or locked disposable loading unit can be removed from the distal end of elongated body 14 by rotating disposable loading unit 16 in the direction opposite to the direction indicated by arrow "B" in FIGS. 41, 42 and 44, to disengage hook portion 258 of second articulation link 256 from finger 164 of first articulation link 123, and to disengage nubs 254 from within channel 314 of elongated body 14. After rotation, disposable loading unit 16 can be slid in the direction opposite to that indicated by arrow "A" in FIG. 41 to detach body 14 from

disposable loading unit **16**. Subsequently, additional articulating and/or non-articulating disposable loading units can be secured to the distal end of elongated body, as described above, to perform additional surgical stapling and/or cutting procedures. As discussed above, each disposable loading unit may include linear rows of staples which vary from about 30 mm to about 60 mm.

Although the above-described surgical stapling instruments may be suitable for their intended purpose, improvements to these instruments are provided below. As described above, surgical stapling instruments can include a handle portion, an elongated body, or shaft, and a disposable loading unit, wherein the disposable loading unit can be removably attached to the elongated body. As described above in connection with disposable loading unit **16** illustrated in FIGS. **40-42**, elongated body **14** of the surgical stapling instrument can define an axis along which disposable loading unit **16** can be assembled thereto. In various circumstances, though, disposable loading unit **16** can become unintentionally detached from elongated body **14** causing the surgical stapling instrument to malfunction or be rendered inoperable. Such circumstances can particularly arise when the disposable loading unit becomes detached and separated from the elongated body along the axis defined by the elongated body, i.e., the axis along which the disposable loading unit was assembled to the elongated body. In various embodiments of the present invention, a disposable loading unit can be assembled to an elongated body of a surgical instrument in a direction which is not collinear with or parallel to the elongated body axis. In at least one embodiment, referring to FIG. **65**, disposable loading unit **1016** can be assembled to elongated body **1014** in a direction which is transverse, perpendicular, or oblique to axis **1015** defined by elongated body **1014**.

In various embodiments, referring to FIGS. **66** and **67**, disposable loading unit **1016** can include connector portion **1017** which can be configured to be engaged with connector portion **1019** of elongated body **1014**. In at least one embodiment, connector portion **1017** can include at least one projection and/or groove which can be mated with at least one projection and/or groove of connector portion **1019**. In at least one such embodiment, the connector portions can include co-operating dovetail portions. In various embodiments, the connector portions can be configured to interlock with one another and prevent, or at least inhibit, distal and/or proximal movement of disposable loading unit **1016** along axis **1015**. In at least one embodiment, similar to the devices described above, the surgical stapling instrument can include control rod **1052** which can be operably connected to drive member **1212** of disposable loading unit **1016** such that drive member **1212** can be advanced distally to deploy staples therefrom and/or incise tissue, for example, upon an actuation of handle member **24** (FIG. **1**). In at least one such embodiment, drive member **1212** can include aperture **1272** which can be configured to receive projection **1276** extending from control rod **1052**. In various embodiments, such an arrangement can allow disposable loading unit **1016** to be assembled to elongated member **1014** in a direction which is not collinear with or parallel to axis **1015**. Although not illustrated, drive member **1212** and control rod **1052** can include any other suitable arrangement of projections and apertures to operably connect them to each other. Also similar to the devices described above, the surgical instrument can include first articulation link **1123** which can be operably engaged with second articulation link **1256** such that the operation of articulation lever **1030** can be transmitted to disposable loading unit **1016**.

In various embodiments, further to the above, the projections and/or grooves of connector portions **1017** and **1019** can be configured such that they can be press-fit together to prevent, or at least inhibit, disposable loading unit **1016** from moving in a direction which is transverse to axis **1015**. In at least one embodiment, referring primarily to FIGS. **68** and **69**, a sleeve, or collar, can be utilized to retain the disposable loading unit to the elongated member. In various embodiments, collar **1021** can be threadably engaged with threaded portion **1023** of disposable loading unit **1016** to prevent connector portions **1017** and **1019** from being disengaged from one another. In at least one embodiment, collar **1021** can include aperture **1025** having, first, a threaded portion **1027** which can threadably engage threaded portion **1023** and, second, a second portion **1029** which can closely receive elongated member **1014** so as to prevent, or at least limit, relative movement between disposable loading unit **1016** and elongated member **1014**. Alternatively, although not illustrated, a collar can be configured to threadably engage elongated member **1014** and closely receive disposable loading unit **1016**. In at least one embodiment, a collar can be configured to threadably engage both the elongated member and the disposable loading unit.

In various embodiments, a detent mechanism can be utilized to retain a disposable loading unit to an elongated member of a surgical stapling instrument. In at least one embodiment, referring to FIGS. **70-72**, elongated member **2014** can include at least one ball detent **2031** which can be configured to engage disposable loading unit **2016** and hold disposable loading unit **2016** in position. In various embodiments, elongated member can include at least one aperture **2033** for receiving ball detents **2031** and at least one retention member **2035** for retaining ball detents **2031** in apertures **2033**. In at least one embodiment, retention members **2035** can also be configured to bias ball detents **2031** into recesses **2037** in disposable loading unit **2016** such that the movement of disposable loading unit **2016** along axis **2015** can be prevented, or at least inhibited. In use, insertion tip **2193** of disposable loading unit **2016** can be inserted into elongated member **2014** such that the end of disposable loading unit **2016** can contact ball detents **2031** and displace them radially within apertures **2033**. Once disposable loading unit **2016** has been inserted to its proper depth, recesses **2037** can be substantially aligned with apertures **2033** and retention members **2035** can position at least a portion of ball detents within recesses **2037**.

In various embodiments, further to the above, at least one of retention members **2035** can be comprised of a resilient material. In at least one embodiment, ball detents **2031** and retention members **2035** can be structured and arranged such that retention members **2035** are deflected outwardly by ball detents **2031** and, as a result, resilient members **2035** can apply a biasing force to ball detents **2031**. In order to release disposable loading unit **2016** from elongated member **2014**, elongated member **2016** can further include actuator **2039** which can be manipulated to retract retention members **2035** proximally such that undercut **2041** of resilient members **2035** can be aligned, or at least substantially aligned, with ball detents **2031**. In various embodiments, the alignment of undercut **2041** with ball detents **2031** can allow ball detents **2031** to be displaced radially and out of engagement with recesses **2037** when disposable loading unit **2016** is pulled out of the aperture in elongated member **2014**. In at least one embodiment, referring to FIGS. **70** and **73**, elongated member **2014** can further include return spring **2043** which can be configured to advance actuator **2039** and retention mem-

bers 2035 distally and reposition retention members 2035 relative to ball detents 2031. In various embodiments, as illustrated in FIGS. 71 and 72, ball detents 2031 can be spherical, or at least substantially spherical, and can be comprised of any suitable material such as stainless steel, for example. In other various embodiments, although not illustrated, detents 2031 can have any suitable non-spherical shape.

In various embodiments, a disposable loading unit and an elongated member of a surgical instrument can include co-operating snap-fit features for retaining the disposable loading unit to the surgical stapling instrument. In at least one embodiment, although not illustrated, a disposable loading unit can include arms extending therefrom which can be at least partially received within apertures or recess in an elongated assembly. In use, the arms can be configured to flex inwardly toward each other as they are inserted into the elongated member and then resiliently spring outwardly when the arms are aligned with the apertures. In various embodiments, the surgical instrument can include a lock which can be slid intermediate the arms to hold the arms in the apertures and prevent, or at least inhibit, the disposable loading unit from becoming detached from the surgical instrument. In at least one embodiment, the lock could be slid distally upon an actuation of a trigger. In various alternative embodiments, the lock can include one or more cams configured to engage the arms and retain them in the apertures when the lock is rotated.

After a disposable loading unit has been attached to a surgical stapling instrument, the instrument can be positioned relative to the soft tissue of a patient. In various circumstances, a surgical stapling instrument can include an anvil and a staple cartridge, where the anvil can be rotated relative to the staple cartridge to position the anvil and the staple cartridge with respect to the soft tissue. As described above in connection with disposable loading unit 16 illustrated in FIGS. 38 and 40, disposable loading unit 16 can include anvil assembly 20 and cartridge assembly 18, where anvil assembly 20 can be pivoted between an open and closed positions. In some such devices, as outlined above and referring to FIG. 24, axial drive assembly 212 can be configured to contact camming surface 209 of anvil assembly 20 and move anvil assembly 20 into a closed position upon a first actuation of movable handle 24. Upon subsequent actuations of movable handle 24, drive assembly 212 can be advanced through disposable loading unit 16 to clamp, staple, and incise the soft tissue positioned intermediate cartridge assembly 18 and anvil assembly 20. In such instruments, as a result of the tissue being clamped at the same time as it is being stapled and incised, a portion of the soft tissue can flow, or 'milk', out of the distal end of the disposable loading unit and, in various circumstances, the soft tissue may not be properly treated by the surgical stapling instrument.

In various embodiments of the present invention, such problems can be ameliorated by utilizing a surgical stapling instrument which can apply a clamping force to soft tissue prior to the staples being deployed from the staple cartridge and/or the drive assembly being advanced within the disposable loading unit. In various circumstances, such embodiments can prevent, or at least inhibit, the soft tissue from milking out of the distal end of the disposable loading unit. In at least one embodiment, a surgical stapling instrument can include an actuator configured to be retracted relative to the distal end of the disposable loading unit to rotate the anvil between an open position and a closed position and clamp the tissue in position. In at least one such

embodiment, referring to FIGS. 74-81, disposable loading unit 3016 can include cartridge assembly 3018 and anvil assembly 3020, where anvil assembly 3020 can be rotated toward cartridge assembly 3018 by actuator 3043. In at least one embodiment, anvil assembly 3020 can include, first, at least one pivot tab 3211 which can be rotatably received within an aperture or recess within staple cartridge assembly 3018, for example, and, second, at least one recess 3047 which can be configured to operably receive at least a portion of actuator 3043. When actuator 3043 is pulled in a direction indicated by arrow "P", in at least one embodiment, actuator 3043 can rotate anvil assembly 3020 into a closed position about an axis defined by pivot tabs 3211 and apply a clamping force to the soft tissue.

In various embodiments, as outlined above, actuator 3043 can include at least one projection 3049 which can be configured to engage the sidewalls of recess 3047 and apply a force to anvil assembly 3020. In at least one embodiment, such a force can generate a torque, or force-moment, causing anvil assembly 3020 to rotate about pivot tabs 3211 between an open position, as illustrated in FIG. 76, and a closed position, as illustrated in FIG. 77. In use, as also outlined above, such a torque can apply a clamping pressure or force to tissue positioned intermediate anvil assembly 3020 and staple cartridge assembly 3018. In various embodiments, the torque applied to anvil assembly 3020 can be directly proportional to the force applied by actuator 3043 and the distance between projections 3049 and pivot tabs 3211, i.e., distance "D" (FIG. 77). In at least one embodiment, a disposable loading unit can be designed such that distance D can be maximized, or at least substantially increased, to apply a larger clamping moment or force to the soft tissue. In at least one such embodiment, referring to FIGS. 80 and 81, staple cartridge assembly 3018 can comprise staple cartridge carrier 3216 which can include apertures, or recesses, 3045 which can be configured to allow at least a portion of projections 3049 to extend therethrough such that the distance between projections 3049 and pivot tabs 3211 can be increased.

In various embodiments, referring to FIG. 75, disposable loading unit 3016 can include spring 3051 which can be configured to bias anvil assembly 3020 into an open position and, in addition, a spring which can bias actuator 3043 into its most distal position. In use, as outlined above, actuator 3043 can be pulled proximally to pivot anvil assembly 3020 into its closed position. In such circumstances, as illustrated in FIG. 77A, anvil assembly 3020 can resiliently compress spring 3051 such that spring 3051 can return anvil assembly 3020 to its open position when actuator 3043 is released as described in greater detail below. In various embodiments, a surgical instrument can include a trigger, or any other suitable actuation device, which can be manipulated by a surgeon, or other clinician, to pull actuator 3043 proximally and, in at least one embodiment, lock actuator 3043 in its retracted position. In at least one embodiment, referring generally to FIGS. 1 and 9, actuator 3043 can be operably engaged with articulation lever 30 and first articulation link 123 such that, when articulation lever 30 is rotated in a first direction, articulation link 123 and actuator 3043 can be retracted proximally. Similarly, when articulation lever 30 is rotated in a second direction, articulation link 123 and actuator 3043 can be advanced distally. In various embodiments, actuator 3043 can be advanced distally to remove projections 3049 from recesses 3047 and allow spring 3051 to return anvil assembly 3020 to its open position.

In various embodiments, a disposable loading unit can include an actuator comprising a cam configured to operably

engage an anvil of the disposable loading unit and apply a compressive pressure or force to soft tissue prior to staples being deployed into the soft tissue. In at least one embodiment, referring to FIGS. 82 and 83, disposable loading unit 4016 can include anvil assembly 4020, staple cartridge assembly 4018, and actuator 4043, where actuator 4043 can be configured to rotate anvil assembly 4020 between an open position, as illustrated in FIG. 82, and a closed position, as illustrated in FIG. 84. In various embodiments, referring to FIGS. 82 and 84, actuator 4043 can include cam 4053 where actuator 4043 can be pulled proximally, i.e., in a direction indicated by arrow "P", such that cam 4053 can engage anvil assembly 4020 and rotate anvil assembly 4020 about an axis defined by pivot tabs 4211. Similar to the above, actuator 4043 can be operable engaged with any suitable trigger, such as articulation lever 30, for example, to motivate actuator 4043.

In various embodiments, an actuator cam can include at least one of a linear, non-linear, arcuate, and/or curvilinear profile. In at least one embodiment, cam 4053 can include an arcuate profile having apex 4055 and initial contact point 4057, for example, where cam 4053 can be configured to engage anvil assembly 4020 such that initial contact point 4057 first contacts anvil assembly 4020. As actuator 4043 is pulled further proximally, cam 4053 can slide relative to anvil assembly 4020 such that various other points of cam 4053 contact anvil assembly 4020 until apex 4055 is in contact with anvil assembly 4020 as illustrated in FIG. 85. At such point, anvil assembly 4020 can be in its closed position. In various embodiments, referring again to FIG. 85, apex 4055 can be positioned proximally relative to pivot tabs 4211, i.e., on the proximal side of axis 4059 and, as a result, anvil assembly 4020 can be prevented from rotating back into its open position until cam 4053 is disengaged from, i.e., moved distally relative to, anvil assembly 4020. Furthermore, the position of apex 4055 relative to pivot tabs 4211 can utilize leverage, or mechanical advantage, to apply an even greater clamping force to the soft tissue.

In various embodiments, as cam 4053 is retracted proximally and anvil assembly 4020 is rotated into its closed position as described above, anvil assembly 4020 can contact soft tissue, for example, positioned intermediate anvil assembly 4020 and staple cartridge assembly 4018. In at least one embodiment, anvil assembly 4020 can apply an initial clamping force to the soft tissue when it initially contacts the tissue and wherein anvil assembly 4020 can apply an increasingly greater force to the soft tissue as anvil assembly 4020 is moved into its final, or closed, position. In various embodiments, the clamping force can be increased in a substantially linear manner. In at least one embodiment, a cam, such as cam 4053, for example, can be configured to drive anvil 4020 in such a manner as to increase the clamping force to the soft tissue in a non-linear manner. In at least one such embodiment, the clamping force can be increased in a geometric manner such that the climax of the clamping force is applied to the soft tissue when anvil assembly 4020 is in its final, or closed, position, for example. As a result of the above, an anvil can apply a clamping force to soft tissue prior to staples being deployed from the staple cartridge, for example, and prevent, or at least inhibit, the soft tissue from flowing, or 'milking', out of the distal end of the disposable loading unit.

In various embodiments, further to the above, a cam can include a profile which utilizes a variable mechanical advantage as the anvil is moved into its closed position. In at least one embodiment, the cam can include a compound profile which includes a first portion for utilizing a first mechanical

advantage, or leverage, during the initial movement of the anvil and, in addition, a second portion for utilizing a second mechanical advantage, or leverage, for subsequent movement of the anvil. In at least one such embodiment, a larger mechanical advantage can be utilized during the final movement of the anvil so as to apply a larger clamping force to the soft tissue when the anvil is in its closed position.

In various embodiments, referring to FIGS. 84 and 85, anvil assembly 4020 can include a tissue-contacting surface, such as surface 4063, for example, which can be positioned parallel to, or at least substantially parallel to, a tissue-contacting surface on staple cartridge assembly 4018, such as surface 4065, for example, when anvil assembly 4020 is in its closed position. In at least one embodiment, anvil assembly 4020 and staple cartridge assembly 4018 can be configured such that there is a gap defined between anvil assembly 4020 and staple cartridge assembly 4018 when anvil assembly 4020 is in its closed position. In various embodiments, the distance between tissue-contacting surfaces 4063 and 4065 can be shorter at distal end 4069 of the disposable loading unit as compared to proximal end 4067. In at least one such embodiment, as a result, the distal end of anvil assembly 4020 can trap soft tissue within the disposable loading unit when anvil assembly 4020 is moved into its closed position. In other various embodiments, the gap between tissue-contacting surfaces 4063 and 4065 can have a consistent, or at least a substantially consistent, distance between proximal end 4067 and distal end 4069.

In various embodiments, referring to FIG. 86, an actuator, such as actuator 4043', for example, can include two or more cams 4053 which can be configured to engage at least a portion of anvil assembly 4020 as described above. In at least one embodiment, cams 4053 can extend from a shaft portion 4061' of actuator 4043' such that cams 4053 can be moved relative to anvil assembly 4020 simultaneously. In various embodiments, actuator 4043' can also include at least one hook portion 258 configured to engage first articulation link 123 as outlined further above. In various alternative embodiments, referring to FIG. 87, a disposable loading unit can include two or more actuators, such as actuators 4043", for example, which can each include one or more cams 4053, for example, for pivoting anvil assembly 4020. In at least one such embodiment, each actuator 4043" can include a hook portion 258 which can be operably connected with one or more articulation links, for example, in a surgical stapling instrument.

In various embodiments of the present invention, a surgical stapling instrument can include a disposable loading unit comprising a staple cartridge, an anvil, and a sleeve, wherein the sleeve can be configured to be slid relative to the staple cartridge and the anvil and hold at least one of the anvil and the staple cartridge in position. In at least one embodiment, referring to FIGS. 109 and 110, disposable loading unit 5016 can include at least one sleeve or collar, such as sleeve 5071, for example, which can be slid between a proximal position, as illustrated in FIG. 109, and a distal position, as illustrated in FIG. 110. In at least one embodiment, sleeve 5071 can include an aperture which, when sleeve 5071 is positioned in its distal position, for example, can at least partially encompass or surround anvil assembly 5020 and/or staple cartridge assembly 5018. In various embodiments, sleeve 5071 can be configured to prevent anvil assembly 5020 from prematurely opening. Furthermore, sleeve 5071 can prevent, or at least inhibit, anvil assembly 5020 and staple cartridge assembly 5018 from deflecting when the soft tissue positioned therebetween is stapled and/or incised.

In at least one embodiment, sleeve **5071**, for example, can be configured to apply a clamping pressure or force to the soft tissue positioned between anvil assembly **5020** and staple cartridge assembly **5018**. In various embodiments, similar to the above, such a clamping pressure or force can be applied before surgical staples are deployed from the staple cartridge and/or the soft tissue is incised. In various embodiments, referring again to FIGS. **109** and **110**, sleeve **5071** can further include slots **5079** which can be configured such that, when sleeve **5071** is advanced distally, sleeve **5071** may not contact and/or damage the tissue positioned between anvil assembly **5020** and staple cartridge assembly **5018**.

In various embodiments, a surgical stapling instrument can include a cantilever, or tongue, configured to be slid relative to at least one of a staple cartridge and an anvil and engage at least one of the staple cartridge and anvil to hold them in a closed position, for example. In at least one embodiment, referring to FIGS. **111** and **112**, disposable loading unit **6016** can include at least one sleeve or collar, such as sleeve **6071**, for example, which can be slid between a proximal position, as illustrated in FIG. **111**, and a distal position, as illustrated in FIG. **112**. In at least one embodiment, sleeve **6071** can include tongue **6073** extending therefrom which can be configured to engage at least a portion of anvil assembly **6020** and apply a force thereto. In various embodiments, such a force can position anvil assembly **6020** against the soft tissue positioned intermediate anvil assembly **6020** and staple cartridge assembly **6018** and clamp the soft tissue therebetween. Referring to FIG. **113**, tongue **6073**, for example, can comprise any suitable configuration including an arcuate, linear, and/or curvi-linear configuration. In at least one embodiment, tongue **6073** can include a curved body comprising proximal end **6075** connected to sleeve **6071** and a distal tip **6077** which can be configured to engage anvil assembly **6020** within anvil cavity **6210**. In at least one such embodiment, the force transmitted between tongue **6073** and anvil assembly **6020** can be applied to anvil assembly **6020** through tip **6077** and, as a result, the location in which the force is applied to the soft tissue can be dictated by the position of tip **6077**.

In various embodiments, sleeve **6071** can be configured such that it can be advanced between its proximal and distal positions prior to staples being deployed from staple cartridge assembly **6018** and the tissue being incised by drive member **6212**, for example. In at least one such embodiment, referring to FIG. **113**, tongue **6073** can be slid distally by sleeve **6071** until distal tip **6077** of tongue **6073** contacts anvil assembly **6020** at distal end **6069**. Thereafter, similar to the above, drive assembly **6212** can be advanced toward the distal end of the disposable loading unit to staple and/or incise the tissue. In such circumstances, the clamping force applied to the soft tissue by tongue **6073** can be applied at the distal end of the disposable loading unit and the possibility that the tissue may milk out of the distal end of the disposable loading unit can be reduced. In other various embodiments, distal tip **6077** can be advanced toward distal end **6069** as drive member **6212** is advanced toward distal end **6069**, for example. In at least one embodiment, distal tip **6077** can be configured to contact anvil assembly **6020** at a location which is positioned directly over, or at least adjacent to, knife blade **6280**. In such embodiments, tongue **6073** can support anvil assembly **6020** directly above the location in which staples are deformed against anvil assembly **6020**.

After an anvil of a disposable loading unit has been moved into a closed position, as outlined above, a drive beam can be advanced within the disposable loading unit to

eject the staples therefrom and/or incise soft tissue. In various embodiments, a drive beam, such as drive beam **266**, for example, can be comprised of a single sheet of material and/or multiple stacked sheets of material. As also outlined above, a drive assembly, such as drive assembly **212**, for example, can further comprise a cam roller **286** and a support member **287** which can be configured to retain drive beam to anvil assembly **20** and staple cartridge assembly **18**, respectively. In various circumstances, the time and cost to assemble such components to drive beam **266** can be significant. In various embodiments of the present invention, such time and cost can be reduced. More particularly, in at least one embodiment of the present invention, a portion of a drive beam can be deformed, or otherwise integrally formed, so as to create features which can obviate the need for a separately-manufactured cam roller **286** and/or support member **287**, for example. In various embodiments, referring to FIGS. **88-90**, drive beam **1266** can include integral cam members **1286** which can extend laterally from retention flange **1284**. In at least one embodiment, drive beam **1266** can be manufactured from a flat, or at least substantially flat, piece of material where the piece of material can be stamped such that cam members **1286** are at least partially separated from retention flange **1284** and extend in a transverse or oblique direction with respect to drive beam **1266**. In at least one such embodiment, referring to FIG. **90**, cam members **1286** can be sized and configured such that they can slide within anvil channel **1210** and at least assist in holding anvil assembly **1020** in a closed position. In addition to or in lieu of the above, although not illustrated, a portion of drive beam **1266**, for example, can be configured to extend laterally from drive beam **1266** so as to retain drive assembly **1212** to a staple cartridge assembly. In at least one embodiment, similar to the above, retention flanges can be at least partially separated from drive beam **1266** during a stamping process such that the integral retention flanges extend in a transverse or oblique direction with respect to drive beam **1266**. In various embodiments, as a result of the above, at least one integral cam member and/or at least one integral retention member can be formed during a suitable manufacturing process, such as progression stamping, for example, which can reduce, or even eliminate, the assembly time of additional components to the drive beam.

In various embodiments, referring to FIG. **49**, the anvil of a disposable loading unit can include a slot defined therein which can be configured to receive at least a portion of a drive beam. In at least one embodiment, referring to FIGS. **51** and **52**, the anvil can include a channel extending therethrough where cam rollers **286** can be configured to engage a sidewall of the channel and apply a force, or forces, to the anvil assembly. In various circumstances, such forces can cause the anvil to elastically and/or plastically deform and, as a result, affect the deployment of the surgical staples into the soft tissue. In various embodiments of the present invention, an anvil can include features which can eliminate, or at least reduce, the deformation of the anvil. In at least one embodiment, an anvil can include a first member having staple pockets for deforming the staples, a first cover plate secured to the first member, and a second cover plate secured to at least one of the first member and the first cover plate, wherein the first and second cover plates can be configured to support the first member. In at least one such embodiment, referring to FIGS. **91-93**, disposable loading unit **7016** can include anvil assembly **7020** which can comprise anvil portion **204**, first cover plate **208** affixed to anvil portion **204**, and second cover plate **7081** affixed to at least one of anvil portion **204** and first cover plate **208**. In various embodi-

ments, first cover plate **208** can be welded to anvil portion **204** and, in addition, second cover plate **7081** can be welded to first cover plate **208** and/or anvil portion **204**. In at least one embodiment, second cover plate **7081** can strengthen, stiffen, and/or increase the section modulus of the anvil assembly, thereby reducing the possibility that the anvil assembly may unsuitably deform during use.

In various embodiments, referring to FIG. **91**, first cover plate **208** can include tissue stops **208'** extending therefrom. In at least one embodiment, tissue stops **208'** can be configured such that, when the anvil and staple cartridge assemblies are positioned relative to soft tissue, tissue stops **208'** can prevent, or at least inhibit, the soft tissue from progressing past a certain point in the disposable loading unit. In various embodiments of the present invention, referring to FIG. **94**, second cover plate **7081a** of disposable loading unit **7016a** can include tissue stops **7081'** extending therefrom in addition to or in lieu of the above. In various embodiments, a disposable loading unit can include a second cover plate which can be formed from one or more sheets of material. In at least one embodiment, referring to FIG. **95**, disposable loading unit **7061b** can include second cover plate **7081b**, wherein second cover plate **7081b** can be formed from a single sheet of material, such as stainless steel, for example. In various embodiments, the sheet of material can be deformed over one or more forming anvils, or mandrels, until it is bent into a suitable shape. In at least one embodiment, the sheet of material can include one or more side edges **7083b** which can be positioned against or proximal to central portion **7085b** of second cover plate **7081b** during the bending process. Thereafter, in at least one such embodiment, side edges **7083b** can be affixed to central portion **7085b** by any suitable manufacturing process, such as welding, for example. As a result of the above, in various embodiments, second cover plate **7081b** can include at least one tissue-contacting edge **7087b** which is formed at the bend between two portions of the sheet material. In at least one such embodiment, the tissue-contacting edges **7087b** can have a rounded or radiused profile which can be configured such that the edges do not damage soft tissue. In various embodiments, further to the above, an anvil can be formed from a sheet of material wherein the formed anvil can include a central portion having a first side and a second side and at least two flaps oppositely folded to one another with one flap on the first side and one flap on the second side.

In various embodiments, referring to FIG. **95**, first cover plate **208** and anvil member **204** can define anvil cavity **210** therebetween. In at least one embodiment, as described above, cavity **210** can be configured to receive cam actuators **286** and, in various circumstances, first cover plate **208** can be configured such that there are large gaps between cam actuators **286** and the sidewalls of cavity **210**. In such an embodiment, however, the configuration of first cover plate **208** may not be optimized so as to maximize the moment of inertia of the anvil assembly with respect to axis **7089b**, for example. As known in the art, a device having a larger moment of inertia with respect to an axis can be more resistant to bending or deformation with respect to that axis. Thus, in various embodiments of the present invention, a cover plate of an anvil assembly can be configured such that the gaps between cam actuators **286** and the cover plate can be eliminated, or at least reduced. In at least one embodiment, referring to FIG. **96**, first cover plate **7208c** can include at least one base portion **7093c** and at least one side wall **7095c** positioned adjacent to, or in abutting contact with, cam actuators **286**. In such embodiments, side walls **7095c** can extend in a direction so as to increase the moment

of inertia of first cover plate **7208c** with respect to axis **7089b**. In various embodiments, side wall portions **7095c** can be oriented in perpendicular, or at least substantially perpendicular, directions with respect to base portions **7093c**.

In various embodiments, further to the above, an anvil assembly can include a first and/or second cover plate which can include ribs and/or folds therein which can strengthen or stiffen the anvil assembly. In at least one embodiment, referring to FIG. **97**, an anvil assembly of disposable loading unit **7016d** can include anvil portion **204** and cover plate **7208d** attached to anvil portion **204**. In various embodiments, cover plate **7208d** can include ribs or folds **7097d** which can increase the moment of inertia of cover plate **7208d** with respect to axis **7089b**. In at least one embodiment, cover plate **7208d** can be manufactured from one or more sheets of material, such as stainless steel, for example, where the sheet, or sheets, can be bent into the configuration illustrated in FIG. **97**. As known in the art, the moment of inertia of a cross-section can be increased by increasing the mass of the cross-section and/or increasing the distance between a mass and a reference axis. The ribs and/or folds **7097d**, as they can add additional mass at a distance from axis **7089b**, can add to the moment of inertia of cover plate **7208d** as compared to cover plate **208**, for example.

In various embodiments, as described above, two or more components of an anvil assembly can be welded together. In at least one embodiment of the present invention, two or more components of an anvil assembly can be press-fit together such that the components are retained to one another. In various embodiments, referring to FIGS. **98-101**, anvil assembly **8020** can include insert portion **8099** and cover portion **8101** where, referring to FIGS. **98** and **100**, insert portion **8099** can be positioned within cavity **8103** defined by cover portion **8101**. Thereafter, referring to FIG. **101**, at least a portion of cover portion **8101** can be deformed, stamped, or swaged such that at least a portion of insert portion **8099** is captured within cavity **8103**. In at least one embodiment, insert portion **8099** can include uneven, rough, and/or corrugated surfaces which can be configured to interlock with portions of cover portion **8101** when it is deformed.

In various embodiments, referring to FIG. **100**, cavity **8103** can include slots or grooves **8105** which can be configured to slidably receive tines **8107** of insert portion **8099** therein, wherein cover portion **8101** can be deformed to capture tines, or arms, **8107** in grooves **8105**. In at least one embodiment, arms **8107** can be press-fit into grooves **8105** where, in various circumstances, such a press-fit can be sufficient to retain insert portion **8099** within cover portion **8101**. In various embodiments, the cover and insert portions of the anvil assembly can be constructed from the same material or different materials. In at least one embodiment, the cover portion can be comprised of a softer or more malleable material than the insert portion. In at least one such embodiment, the cover portion can be at least partially comprised of aluminum, for example, and the insert portion can be at least partially comprised of steel, for example. In either event, the cover portion can be comprised of a material which can be stamped or coined to form the staple-deforming pockets therein. In at least one such embodiment, the cover portion can then be anodized.

In various embodiments, as described above, an anvil assembly can comprise an anvil portion have staple-deforming pockets therein and a cover plate for supporting the anvil portion. In at least one embodiment, the anvil portion and the cover plate can be integrally formed. Referring to FIGS.

**102-103**, anvil **8020a** can be manufactured from a tube, or annulus, of material where, in at least one embodiment, at least a portion of the tube, such as portion **8109a**, for example, can be removed. In at least one such embodiment, the remaining portion of the tube, such as portion **8111a**, for example, can be deformed utilizing a stamping or forming process such that anvil **8020a** can include co-planar, or at least substantially co-planar, anvil portions **8204a** extending from support portion **8208a**. In various embodiments, the tube can be at least partially comprised of extruded aluminum and, in at least one embodiment, staple-deforming cavities **206** can be formed in the tube prior to and/or after the portion of the tube is removed.

In various embodiments, as described above, an anvil assembly can be comprised of two or more components which are press-fit together. In at least one embodiment, referring to FIGS. **105** and **106**, anvil assembly **8020b** can include a first, or insert, portion **8099b** and a second, or cover, portion **8101b**, wherein insert portion **8099b** can be inserted into cavity **8103b** of cover portion **8101b**. In at least one embodiment, the outer surface of insert portion **8099b** can define a perimeter which is larger than a perimeter defined by an outer surface of outer portion **8101b** wherein, as a result, insert portion **8099b** can expand outer portion **8101b** outwardly when insert portion **8099b** is inserted into cavity **8103b**. Owing to such co-operating geometries, a significant normal force can be generated between the surfaces of portions **8099b** and **8101b**. In at least one such embodiment, as a result, a significant pulling force may be required to overcome the friction force between members **8099b** and **8101b** resulting from the high normal force therebetween.

In various embodiments, an anvil assembly can be comprised of two or more components which are snap-fit together. In at least one embodiment, referring to FIGS. **106-108**, anvil assembly **8020c** can include first portion **8099c** and second portion **8101c**, where second portion **8101c** can be snap-fit to first portion **8099c**. Referring to FIG. **109**, in at least one embodiment, second portion **8101c** can include projections **8113c** extending therefrom which can be configured to fit within grooves **8115c**. In various embodiments, second portion **8101c** can be at least partially comprised of a resilient material, such as stainless steel, for example, which can allow projections **8113c** to be displaced outwardly as surface **8117c** of second portion **8101c** is moved toward surface **8119c** of first portion **8099c**. Once surface **8117c** is positioned against or adjacent to surface **8119c**, projections **8113c** can be resiliently positioned within, or snapped into, grooves **8115c** such that second portion **8101c** is retained to first portion **8099c**. In at least one embodiment, the first and second portions can be comprised of the same material or they can be comprised of different materials. In at least one embodiment, first portion **8099c** can be at least partially comprised of aluminum and second portion **8101c** can support the first portion.

In various embodiments, referring to FIG. **86**, an anvil can include an anvil member, such as anvil member **4204**, for example, which can include ribs or ridges **4153** extending therefrom. In at least one embodiment, ribs **4153** can increase the moment of inertia or cross-sectional modulus of anvil member **4204**, for example, such that anvil assembly **4020** is less susceptible to unwanted deformation. In various embodiments, ribs **4153** can extend around the perimeter of anvil member **4204**.

In various embodiments, although not illustrated, other components can be assembled to an anvil. In at least one embodiment, a soft or pliable nosepiece, for example, can be

assembled to the anvil in order to reduce the possibility that the anvil may damage soft tissue when it is inserted into a surgical site. In at least one such embodiment, the nosepiece, or any other suitable component, can be comprised of any suitable material such as rubber and/or nylon, for example.

In various embodiments, as described above, cam actuators **286**, for example, can be configured to engage an anvil assembly and position the anvil assembly against soft tissue positioned intermediate the anvil assembly and a staple cartridge. In at least one embodiment of the present invention, referring to FIGS. **104** and **105**, anvil assembly **8020b**, for example, can include contact surface, or surfaces, **8121b**, wherein cam actuators **286** can be configured to engage contact surfaces **8121b** and hold anvil assembly **8020b** in a closed position. In various embodiments, contact surfaces **8121b** can be configured such that they extend inwardly toward drive beam **1266** such that at least a portion of the contact surfaces are positioned adjacent to, or in contact with, drive beam **1266**. In at least one embodiment, as a result, contact surfaces **8121b** can be configured such that the contact area between cam actuators **286** and contact surfaces **8121b** can be maximized, or at least increased. As a result of the increased contact area, the stress or pressure applied by actuators **286** to contact surfaces **8121b** can be reduced and the possibility of galling and/or localized yielding of the anvil assembly can be reduced.

In various circumstances, especially during endoscopic or laparoscopic surgical procedures, for example, at least a portion of a surgical stapling instrument can be inserted through a cannula, or trocar, into a surgical site. Often, an anvil of a disposable loading unit is moved into its closed position before it is inserted into the trocar and then reopened after it has been inserted therethrough. Some disposable loading units having large anvils and/or staple cartridges may not fit, or easily fit, through the trocar even when the anvil is in the closed position. In various embodiments of the present invention, a surgical stapling instrument can include a disposable loading unit having an anvil which can be moved between open, closed, and/or collapsed positions to facilitate the insertion of the disposable loading unit through the trocar. More particularly, in at least one embodiment, an anvil can be moved into a closed position in which the anvil is a first distance away from the staple cartridge, for example, and a collapsed position in which the anvil is closer to the staple cartridge such that the disposable loading unit can be more easily inserted through the trocar.

In various embodiments of the present invention, further to the above and referring to FIGS. **114-116**, a disposable loading unit **9016** can include anvil assembly **9020** and staple cartridge assembly **9018**, wherein anvil assembly **9020** can be rotatably mounted relative to staple cartridge assembly **9018**. In use, similar to the above, drive assembly **212** can be advanced distally such that cam actuators **286** can contact anvil member **9204** and rotate anvil assembly **9020** between an open position, as illustrated in FIGS. **115** and **116**, and a closed position, as illustrated in FIGS. **117** and **118**. When anvil assembly **9020** is rotated toward staple cartridge assembly **9018**, in at least one embodiment, anvil assembly **9020** can be configured to compress at least one return spring **9051**, for example, in the disposable loading unit.

In at least one embodiment, referring to FIG. **118**, anvil assembly **9020** can further include tissue-contacting surface **9020'** and, similarly, staple cartridge assembly **9018** can include tissue contacting surface **9018'**. In various embodiments, tissue-contacting surfaces **9018'** and **9020'** can be separated by a first distance **9121** when anvil assembly **9020**



is in a closed position. In order to move anvil assembly **9020** into a collapsed position, in various embodiments, actuator **9043** can be moved distally, for example, such that portion **9049** of actuator **9043** can contact anvil assembly **9020** and push anvil assembly **9020** toward staple cartridge assembly **9018** as illustrated in FIGS. **119** and **120**. In such a collapsed position, in at least one embodiment, tissue-contacting surfaces **9018'** and **9020'** can be separated by a second distance **9125** which can be shorter than first distance **9121**. In various embodiments, actuator **9043** can push anvil assembly **9020** downwardly until surface **9020'** at least partially abuts surface **9018'**.

In various embodiments, further to the above, a disposable loading unit can include at least one return spring which can be compressed when the anvil assembly is moved into its collapsed position. In at least one embodiment, referring to FIGS. **116** and **118**, disposable loading unit **9016** can include springs **9123** which can be compressed when anvil assembly **9020** is moved between its open and closed positions and, referring to FIGS. **118** and **120**, further compressed when anvil assembly is moved into its collapsed position. Once the anvil assembly is in its collapsed position, the disposable loading unit can be inserted into a trocar, which is represented in dash as circle **9155** in FIG. **121**. After at least a portion of anvil assembly **9020** and staple cartridge assembly **9018** have passed through the trocar, actuator **9043** can be disengaged from anvil assembly **9020** to allow springs **9123** to move anvil assembly from its collapsed position into its closed position, as illustrated in FIG. **122**. Furthermore, cam actuators **286** can be sufficiently disengaged from anvil assembly **9020** to allow springs **9051** to move anvil assembly **9020** into its open position such that the anvil and staple cartridge assemblies can be positioned relative to soft tissue.

In various embodiments, as outlined above, cam actuators **286** can be utilized to move anvil assembly **9020** between an open position and a closed position and, thereafter, actuator **9043** can be utilized to move anvil assembly **9020** between the closed position and a collapsed position. Alternatively, actuator **9043** can be configured such that it can engage anvil assembly **9020** when it is in its open position and move anvil assembly **9020** directly into its collapsed position. In various circumstances, such embodiments can allow a surgeon to more quickly and easily configure a disposable loading unit to be inserted through a trocar. In at least one such embodiment, after at least a portion of the anvil assembly has been inserted through the trocar, the actuator can be sufficiently disengaged from the anvil assembly such that the anvil assembly can be moved directly into its open position and positioned relative to soft tissue, for example. In order to remove the disposable loading unit from the surgical site, the actuator can be reengaged with the anvil assembly to move the anvil assembly into its collapsed position such that the disposable loading unit can be withdrawn through the trocar.

With respect to the disposable loading units and surgical instruments described further above, referring to FIGS. **41** and **42**, a disposable loading unit can be inserted into the distal end of a surgical instrument and can be rotated with respect to the surgical instrument in order to operably engage the drive assembly and/or articulation link of the disposable loading unit with the surgical instrument. In at least one embodiment of the present invention, such rotation can unlock the drive assembly and allow the drive assembly to be advanced distally as described above. Referring to FIG. **123**, disposable loading unit **10016** can include anvil assembly **10020**, shaft assembly **10125**, and lockout device **10127**, where lockout device **10127** can be engaged with

drive assembly **10212** (FIG. **128**) prior to disposable loading unit **10016** being rotated relative to elongated body **14** (FIG. **1**) of the surgical instrument. In at least one such embodiment, referring to FIG. **124**, lockout device **10127** can include key **10131** which can be configured to engage a recess in drive assembly **10212**, for example, so as to prevent, or at least inhibit, drive assembly **10212** from being advanced distally prior to disposable loading unit **10016** being rotated. As disposable loading unit **10016** is rotated, key **10131** can be disengaged from drive assembly **10212** and, as a result, drive assembly **10212** can be advanced distally as described above.

In various embodiments, referring to FIGS. **123** and **124**, lockout device **10127** can include arms **10129** extending therefrom which, prior to the rotation of disposable loading unit **10016**, can be aligned, or at least substantially aligned, with nubs **254** extending from shaft assembly **10125**. In at least one embodiment, referring to FIGS. **125** and **126**, arms **10129** and nubs **254** can be inserted into slots **10133** in elongated body **14**, for example, when disposable loading unit **10016** is inserted into elongated body **14**. When disposable loading unit **10016** is rotated, referring to FIG. **127**, arms **10129** can be sufficiently confined within slots **10133** such that slots **10133** can hold them in position, whereas nubs **254** can be positioned such that they are not confined within slots **10133** and can be rotated relative to arms **10129**. In effect, elongated body **14** can hold lockout device **10127** in position and, when shaft assembly **10125** is rotated with disposable loading unit **10016**, drive assembly **10212** can be rotated away from key **10131** of lockout device **10127**.

To detach disposable loading unit **10016** from elongated member **14**, disposable loading unit **10016**, and shaft assembly **10125**, can be rotated in an opposite direction such that nubs **254** are at least substantially realigned with arms **10129** and, as a result, nubs **254** and arms **10129** can be withdrawn from slots **10133**. Such circumstances can typically arise after the disposable loading unit has been used, or expended, and the surgeon, or other clinician, desires to assemble a new disposable loading unit to the elongated body. In various circumstances, though, the surgeon, or other clinician, may become confused as to whether a disposable loading unit has been previously expended. In various embodiments of the present invention, the lockout device described above, or any other suitable lockout device disclosed herein, can be utilized to prevent, or at least inhibit, an expended disposable loading unit from being reassembled to the elongated body of the surgical instrument.

In various embodiments, referring to FIG. **128**, disposable loading unit **10016** can further include biasing spring **10135**, actuator **10137**, and actuator plate **10139** extending from actuator **10137**, wherein actuator plate **10139** can be configured to operably engage spring **10135**. After disposable loading unit **10016** has been operably engaged with elongated portion **14**, as described above, drive assembly **10212** can be advanced distally to staple and/or incise tissue. In at least one embodiment, actuator **10137** can be operably attached to drive assembly **10212** such that, when drive assembly **10212** is advanced, drive assembly **10212** can pull actuator **10137** and actuator plate **10139** distally as well. Once drive assembly **10212** has been sufficiently advanced, referring to FIG. **129**, actuator plate **10139** can be sufficiently disengaged from biasing spring **10135** so as to release biasing spring **10135** from a compressed state and allow biasing spring **10135** to apply a biasing force against lockout device **10127**. However, at such point, as lockout device **10127** is held in position by elongated member **14**, as described above, the biasing force applied by spring **10135**

cannot move, or at least substantially move, lockout device **10127**, at least as long as disposable loading unit **10016** remains engaged with elongated member **14**.

In various embodiments, the disengagement of actuator plate **10139** from biasing spring **10135** can occur before, or at the exact moment, in which a staple can be deployed from the staple cartridge and/or the cutting member can incise the tissue. In at least one such embodiment, a surgeon could advance and retract drive assembly **10212** in order to position anvil assembly **10020** relative to soft tissue without triggering the lockout assembly described above. After actuator **10137** has been sufficiently advanced to disengage plate **10139** from spring **10135**, drive assembly **10212** can be further advanced distally such that, referring again to FIG. **129**, actuator **10137** and/or actuator plate **10139** can abut a shoulder, for example, within the disposable loading unit. In at least one such embodiment, the shoulder can prevent actuator **10137** and actuator plate **10139** from being advanced further within the disposable loading unit. Upon further advancement of drive assembly **10212**, however, actuator **10137** can become operably detached from drive assembly **10212** such that the advancement of drive assembly **10212** is not transmitted to actuator **10137**.

After disposable loading unit **10016** has been disengaged from elongated member **14**, referring to FIG. **130**, biasing spring **10135** can move, or rotate, locking device **10127** into a position in which arms **10129** are no longer aligned with nubs **254**. In at least one such embodiment, such a disposable loading unit **10016** cannot be readily reassembled to elongated member **14** as arms **10129** and nubs **254** would not both fit within slots **10133** owing to their relative misalignment. In various embodiments, such disposable loading units can provide the surgeon, or other clinician, with immediate feedback that they are attempting to assemble an expended, or possibly defective, disposable loading unit to a surgical instrument. Such embodiments can ameliorate the circumstances where an at least partially expended disposable loading unit is reassembled to a surgical instrument and reinserted into a surgical site only for the surgeon to then discover that the disposable loading unit has been expended. In various embodiments, drive assembly **10212** and actuator **10137** can be configured such that, in the event that drive assembly **10212** is retracted, drive assembly **10212** may not cause actuator **10137** to reengage biasing spring **10135** and return biasing spring **10135** to its compressed state.

In various embodiments, referring primarily to FIG. **126**, slots **10133** of elongated member **14** can include a substantially rectangular profile which extends along the length thereof. While suitable for its intended purpose, circumstances may arise where it may be difficult to assemble the disposable loading unit to the elongated member. More particularly, in at least one embodiment, the disposable loading unit can be configured such that a surgeon, or other clinician, can not readily observe whether nubs **254** are aligned with slots **10133** and the surgeon may have spent time to precisely align nubs **254** with slots **10133** before assembling the disposable loading unit to elongated member **14**. In at least one embodiment of the present invention, referring to FIG. **64**, elongated member **14'** can include slots **10133'** having radiused and/or beveled ends **10141'** which can facilitate the insertion of nubs **254** into slots **10133'** and reduce the time and/or effort that a surgeon must expend to align and assemble the disposable loading unit to the surgical instrument.

As described above, a disposable loading unit can be detached from a surgical instrument after it has been at least

partially expended and a new disposable loading unit can be attached to the surgical instrument such that the surgical instrument can be reused. In various embodiments, previous disposable loading units have included a housing, an anvil assembly, and a staple cartridge assembly, as outlined above, and, in addition, a staple driver for deploying staples from the staple cartridge assembly and a cutting member for incising tissue. When the staple cartridge assemblies of such disposable loading units are at least partially expended, the remainder of the disposable loading unit, such as the housing, the anvil assembly, the staple driver, and the cutting member, for example, are typically discarded along with the expended staple cartridge assembly. As a result, significant cost and undue waste can be expended to replace such previous disposable loading units.

In various embodiments of the present invention, a disposable loading unit can include a replaceable staple cartridge. In at least one embodiment, referring to FIGS. **131-135**, disposable loading unit **11016** can include anvil assembly **11020**, staple cartridge channel **11216**, and staple cartridge **11018**, wherein staple cartridge **11018** can be removably attached to staple cartridge channel **11216**. In at least one embodiment, as a result, a first staple cartridge **11018** can be replaced with a second staple cartridge **11018**, or another suitable staple cartridge, such that one or more of the various other portions of the disposable loading unit can be reused. In various embodiments, referring to FIG. **132**, staple cartridge **11018** can be snap-fit into staple cartridge channel **11216** such that staple cartridge **11018** can be reliably retained within, yet easily removed from, staple cartridge channel **11216**.

In at least one embodiment, staple cartridge **11018** can include body portion **11143** having at least one staple cavity for removably storing at least one staple therein and, in addition, cartridge pan **11145** which can be attached to body portion **11143**. In various embodiments, cartridge pan **11145** can be snap-fit and/or press-fit to body portion **11143** to prevent, or at least inhibit, the staples within the staple cavities from falling out of the bottom of body portion **11143**. In at least one embodiment, body portion **11143** and/or cartridge pan **11145** can include one or more projections **11147** and/or apertures **11149** which can be configured to retain body portion **11143** and cartridge pan **11145** to one another. In various embodiments, cartridge pan **11145** can further include projections or dimples **11151**, for example, which can be configured to engage staple cartridge channel **11216** and retain staple cartridge **11018** thereto.

In various embodiments, as described above, staple driver **232** and cutting member **280** can be advanced distally to deploy staples from the staple cartridge and incise soft tissue. Thereafter, in at least one embodiment of the present invention, staple driver **232** and cutting member **280** can be retracted relative to the staple cartridge such that, when the staple cartridge is replaced, staple driver **232** and cutting member **280** can be advanced distally once again into the new staple cartridge. In various embodiments, the staple driver and/or cutting member can remain in the spent staple cartridge as the staple cartridge is being removed and the new staple cartridge can include a new staple driver positioned therein. In at least one such embodiment, each staple cartridge can include a staple driver and a cutting member positioned therein such that the staple driver and cutting member of a spent staple cartridge do not have to be reused. Such embodiments can be useful when the staple driver and the cutting member can be damaged and/or dulled during their use. In various embodiments, the staple driver and the cutting member can comprise an assembly. In at least one

such embodiment, the cutting member can be snap-fit and/or press-fit into the staple driver. In other embodiments, the cutting member can be comprised of a plastic material, for example, which is overmolded onto the cutting member.

As described above, an anvil assembly of a disposable loading unit can include one or more pockets therein for deforming at least one staple when it is ejected from the staple cartridge. In various embodiments of the present invention, an anvil can be attached to the disposable loading unit such that it cannot be readily detached from the disposable loading unit even though the staple cartridge may be readily removable. In various circumstances, however, the anvil may become worn after a single use and/or multiple uses. In at least one embodiment of the present invention, at least a portion of an anvil assembly can be configured such that it can be detached from disposable loading unit and replaced with a new portion of the anvil assembly. In at least one such embodiment, the anvil assembly and the staple cartridge can both be replaced before a disposable loading unit is reused. In various embodiments, further to the above, a disposable loading unit can include a staple cartridge channel, or at least a portion of a staple cartridge channel, which is detachable from the disposable loading unit. In at least one such embodiment, the staple cartridge channel, or a portion of the staple cartridge channel, can be replaced along with a staple cartridge.

When a staple cartridge and/or anvil of a disposable loading unit is replaced, in various embodiments of the present invention, the staple cartridge and anvil can be replaced with an identical, or at least nearly identical, staple cartridge and anvil. In at least one such embodiment, for example, a 30 mm staple cartridge can be replaced with another 30 mm staple cartridge. In at least one embodiment, however, the staple cartridge and/or anvil can be replaced with a different staple cartridge and anvil. In at least one such embodiment, a 30 mm staple cartridge can be replaced with a 45 mm staple cartridge. Such embodiments may be particularly useful when the anvil assembly and/or staple cartridge channel are also replaced to accommodate the different staple cartridge. Other embodiments are envisioned in which a staple cartridge is replaced with a staple cartridge having a different quantity and/or arrangement of staples stored therein. In such embodiments, similar to the above, at least a portion of the anvil assembly can be replaced to accommodate such a staple cartridge. In various embodiments, sets of anvils and staple cartridges can be provided for and/or with a disposable loading unit. In at least one such embodiment, a rigid anvil can be provided for use with a staple cartridge containing staples which will require a large force to deform the staples. In other various embodiments, an anvil can be provided having specialized staple-deforming pockets which are particularly designed to deform a particular staple, such as staples with long staple legs, for example. In at least one embodiment, the anvil and staple cartridge can include corresponding indicia, such as colors, numbers, and/or symbols, etc. which can allow a surgeon, or other clinician, to readily identify matching pairs of anvils and staple cartridges.

Several of the disposable loading unit embodiments described above have been exemplified with an anvil having a distal end which is movable relative to a distal end of a staple cartridge. In various alternative embodiments, although not illustrated, a disposable loading unit can include an anvil and a staple cartridge wherein the anvil can include a distal end which is pivotably mounted relative to the staple cartridge at its distal end. In at least one embodiment, the disposable loading unit can include an actuator

which can be displaced distally to engage the anvil and rotate the anvil between an open position and a closed position. In at least one such embodiment, the staple cartridge can include a staple cartridge and/or a cutting member which can be displaced from a position located near the distal end of the anvil to a proximal end of the anvil. In at least one such embodiment, as a result, a surgeon can more readily observe whether soft tissue has been properly positioned between and/or treated within the staple cartridge and anvil.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

Preferably, the invention described herein will be processed before surgery. First, a new or used instrument is obtained and if necessary cleaned. The instrument can then be sterilized. In one sterilization technique, the instrument is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and instrument are then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation kills bacteria on the instrument and in the container. The sterilized instrument can then be stored in the sterile container. The sealed container keeps the instrument sterile until it is opened in the medical facility.

It will be understood that various modifications may be made to the embodiments disclosed herein. For example, the stapling apparatus need not apply staples but rather may apply two part fasteners as is known in the art. Further, the length of the linear row of staples or fasteners may be modified to meet the requirements of a particular surgical procedure. Thus, the length of a single stroke of the actuation shaft and/or the length of the linear row of staples and/or fasteners within a disposable loading unit may be varied accordingly. Therefore, the above description should not be construed as limiting, but merely as exemplifications of preferred embodiments. Those skilled in the art will envision other modifications within the scope and spirit of the claims appended thereto.

What is claimed is:

1. A surgical stapling assembly, comprising:
  - a shaft comprising an attachment interface, wherein said surgical stapling assembly is configured to be attached to a surgical instrument interface by way of said attachment interface;
  - a firing member;
  - an end effector extending from said shaft, wherein said end effector comprises:
    - a staple cartridge comprising a plurality of staples configured to be ejected by said firing member;
    - a first jaw;

39

a second jaw movable relative to said first jaw between:  
 an open position;  
 a fully-clamped position; and  
 a collapsed position; and  
 an interconnection between said first jaw and said  
 second jaw defining a rotational axis about which  
 said second jaw is movable relative to said first jaw,  
 wherein said rotational axis is shiftable toward and  
 away from said first jaw as said second jaw is moved  
 between said open position, said fully-clamped posi-  
 tion, and said collapsed position; and  
 a closure member configured to move said second jaw  
 from said open position to said collapsed position when  
 said closure member moves from a proximal position to  
 a distal position.

2. The surgical stapling assembly of claim 1, wherein said  
 proximal position comprises a first proximal position,  
 wherein said closure member is movable from said distal  
 position to a second proximal position to move said second  
 jaw from said collapsed position to said open position, and  
 wherein said first proximal position and said second proximal  
 position are different.

3. A surgical stapling assembly, comprising:  
 a shaft comprising an attachment interface, wherein said  
 surgical stapling assembly is configured to be attached  
 to a surgical instrument interface by way of said  
 attachment interface;  
 a firing member;  
 an end effector extending from said shaft, wherein said  
 end effector comprises:  
 a staple cartridge comprising a plurality of staples  
 configured to be ejected by said firing member;  
 a first jaw; and  
 a second jaw movable relative to said first jaw between:  
 an open position;  
 a fully-clamped position; and  
 a collapsed position; and  
 a closure member configured to move said second jaw  
 from said open position to said collapsed position when  
 said closure member moves from a proximal position to  
 a distal position,  
 wherein said surgical stapling assembly is attached to the  
 surgical instrument interface by way of a twisting  
 motion.

4. A surgical stapling assembly, comprising:  
 a shaft comprising an attachment interface, wherein said  
 surgical stapling assembly is configured to be attached  
 to a surgical instrument interface by way of said  
 attachment interface;  
 a firing actuator;  
 an end effector extending from said shaft, wherein said  
 end effector comprises:  
 a staple cartridge comprising a plurality of staples  
 configured to be ejected by said firing actuator;  
 a first jaw; and  
 a second jaw defining a rotational axis about which said  
 second jaw is movable relative to said first jaw  
 between:  
 an unclamped position defining a first distance  
 between said first jaw and said second jaw;  
 a fully-clamped position defining a second distance  
 between said first jaw and said second jaw; and  
 a closed position defining a third distance between  
 said first jaw and said second jaw, wherein said  
 first distance is greater than said second distance,  
 wherein said second distance is greater than said  
 third distance, and wherein said rotational axis is

40

movable toward and away from said first jaw as  
 said second jaw is moved between said unclamped  
 position, said fully-clamped position, and said  
 closed position; and  
 a closure actuator configured to move said second jaw  
 from said unclamped position to said closed position  
 when said closure actuator moves from a proximal  
 position to a distal position.

5. The surgical stapling assembly of claim 4, wherein said  
 proximal position comprises a first proximal position,  
 wherein said closure actuator is movable from said distal  
 position to a second proximal position to move said second  
 jaw from said closed position to said unclamped position,  
 and wherein said first proximal position and said second  
 proximal position are different.

6. A surgical stapling assembly, comprising:  
 a shaft comprising an attachment interface, wherein said  
 surgical stapling assembly is configured to be attached  
 to a surgical instrument interface by way of said  
 attachment interface;  
 a firing actuator;  
 an end effector extending from said shaft, wherein said  
 end effector comprises:  
 a staple cartridge comprising a plurality of staples  
 configured to be ejected by said firing actuator;  
 a first jaw; and  
 a second jaw movable relative to said first jaw between:  
 an unclamped position defining a first distance  
 between said first jaw and said second jaw;  
 a fully-clamped position defining a second distance  
 between said first jaw and said second jaw; and  
 a closed position defining a third distance between  
 said first jaw and said second jaw, wherein said  
 first distance is greater than said second distance,  
 wherein said second distance is greater than said  
 third distance; and  
 a closure actuator configured to move said second jaw  
 from said unclamped position to said closed position  
 when said closure actuator moves from a proximal  
 position to a distal position,  
 wherein said surgical stapling assembly is attached to the  
 surgical instrument interface by way of a twisting  
 motion.

7. A surgical stapling assembly, comprising:  
 a shaft;  
 a firing member comprising a first clamping member;  
 an end effector extending from said shaft, wherein said  
 end effector comprises:  
 a staple cartridge comprising a plurality of staples  
 configured to be ejected by said firing member;  
 a first jaw; and  
 a second jaw defining a rotational axis about which said  
 second jaw is movable relative to said first jaw  
 between:  
 an unclamped position defining a first distance  
 between said first jaw and said second jaw;  
 a fully-clamped position defining a second distance  
 between said first jaw and said second jaw; and  
 a closed position defining a third distance between  
 said first jaw and said second jaw, wherein said  
 first distance is greater than said second distance,  
 wherein said second distance is greater than said  
 third distance, and wherein said rotational axis is  
 movable toward and away from said first jaw as  
 said second jaw is moved between said unclamped  
 position, said fully-clamped position, and said  
 closed position; and

41

a closure member comprising a second clamping member,  
 wherein said closure member is configured to move  
 said second jaw from said unclamped position to said  
 closed position when said closure member moves from  
 a proximal position to a distal position. 5

8. The surgical stapling assembly of claim 7, wherein said  
 proximal position comprises a first proximal position,  
 wherein said closure member is movable from said distal  
 position to a second proximal position to move said second  
 jaw from said closed position to said unclamped position, 10  
 and wherein said first proximal position and said second  
 proximal position are different.

9. A surgical stapling assembly, comprising:

a shaft;

a firing member comprising a first clamping member; 15

an end effector extending from said shaft, wherein said  
 end effector comprises:

a staple cartridge comprising a plurality of staples  
 configured to be ejected by said firing member;

42

a first jaw; and

a second jaw movable relative to said first jaw between:  
 an unclamped position defining a first distance  
 between said first jaw and said second jaw;

a fully-clamped position defining a second distance  
 between said first jaw and said second jaw; and

a closed position defining a third distance between  
 said first jaw and said second jaw, wherein said  
 first distance is greater than said second distance,  
 and wherein said second distance is greater than  
 said third distance; and

a closure member comprising a second clamping member,  
 wherein said closure member is configured to move  
 said second jaw from said unclamped position to said  
 closed position when said closure member moves from  
 a proximal position to a distal position, 15

wherein said shaft comprises an attachment interface,  
 wherein said surgical stapling assembly is configured to  
 be attached to a surgical instrument interface by way of  
 said attachment interface by way of a twisting motion.

\* \* \* \* \*