



US010847295B2

(12) **United States Patent**  
**Rapoport et al.**

(10) **Patent No.:** **US 10,847,295 B2**  
(45) **Date of Patent:** **\*Nov. 24, 2020**

(54) **DEVICE, SYSTEM AND METHOD FOR OBTAINING A MAGNETIC MEASUREMENT WITH PERMANENT MAGNETS**

(71) Applicant: **Aspect Imaging Ltd.**, Shoham (IL)

(72) Inventors: **Uri Rapoport**, Moshav Ben Shemen (IL); **Yair Goldfarb**, Ness Ziona (IL); **Yoram Cohen**, Yarkona (IL)

(73) Assignee: **ASPECT IMAGING LTD.**, Shoham (IL)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **16/253,584**

(22) Filed: **Jan. 22, 2019**

(65) **Prior Publication Data**

US 2019/0172620 A1 Jun. 6, 2019

**Related U.S. Application Data**

(63) Continuation of application No. 15/402,438, filed on Jan. 10, 2017, now Pat. No. 10,224,135.

(60) Provisional application No. 62/372,065, filed on Aug. 8, 2016, provisional application No. 62/381,079, filed on Aug. 30, 2016.

(51) **Int. Cl.**

**G01V 3/00** (2006.01)  
**H01F 7/02** (2006.01)  
**G01R 33/383** (2006.01)  
**G01R 33/3873** (2006.01)  
**G01R 33/421** (2006.01)

(52) **U.S. Cl.**  
CPC ..... **H01F 7/0278** (2013.01); **G01R 33/383** (2013.01); **G01R 33/3873** (2013.01); **G01R 33/421** (2013.01)

(58) **Field of Classification Search**  
USPC ..... 324/309  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,900,342 A 3/1933 Hess  
2,708,927 A 5/1955 Dixon  
(Continued)

FOREIGN PATENT DOCUMENTS

CA 2815746 5/2012  
CA 2863080 8/2013  
(Continued)

OTHER PUBLICATIONS

Liming Hong and Donglin Zu, Shimming Permanent Magnet of MRI Scanner, Piers Online, 2007, vol. 3, No. 6, 859-864.

(Continued)


*Primary Examiner* — Rodney E Fuller

(74) *Attorney, Agent, or Firm* — Loeb & Loeb

(57) **ABSTRACT**

A magnetic field device, with a first magnet, a first ferromagnetic element positioned adjacent to the first magnet, a second magnet, a second ferromagnetic element positioned adjacent to the second magnet and relative to the first ferromagnetic element to create a gap between the first ferromagnetic element and the second ferromagnetic element, and a third magnet positioned between the first ferromagnetic element and the second ferromagnetic element and within the gap.

**21 Claims, 11 Drawing Sheets**

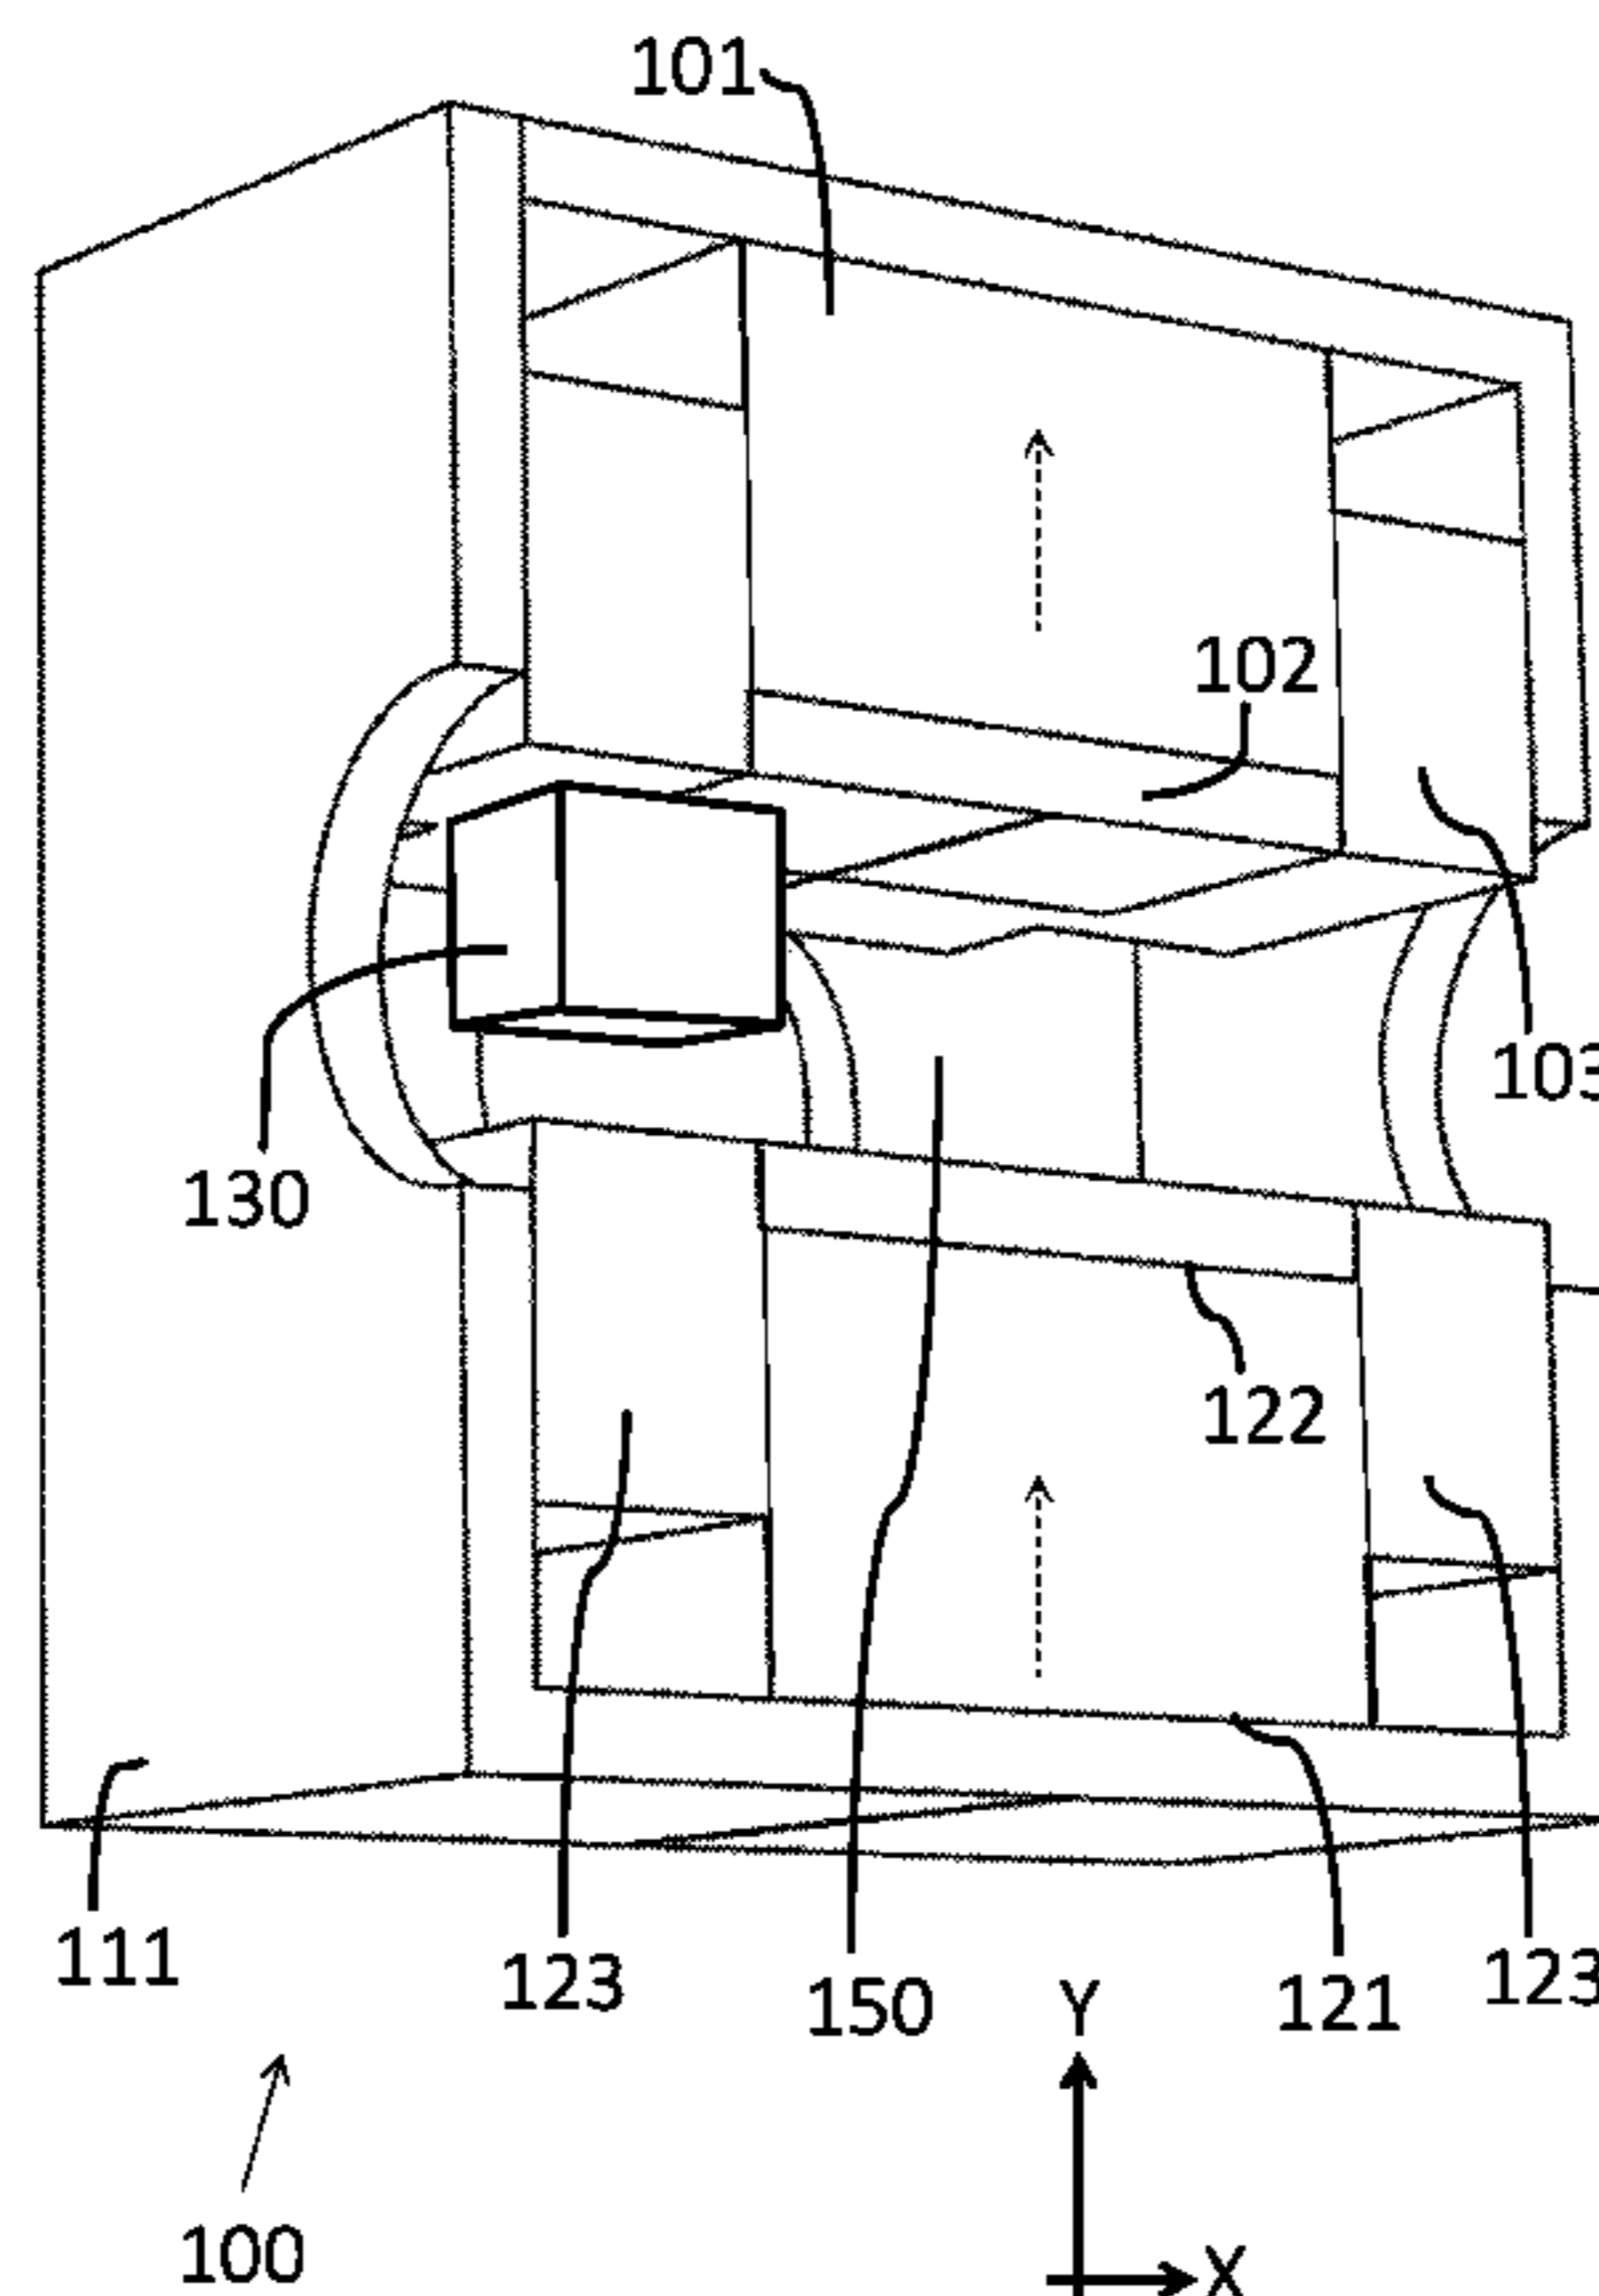

(56)

References Cited

U.S. PATENT DOCUMENTS

3,012,836	A	12/1961	Smith	6,946,939	B2	9/2005	Doi
3,315,671	A	4/1967	Creelman	6,992,486	B2	1/2006	Srinivasan
3,470,866	A	10/1969	Gittelsohn	7,034,530	B2	4/2006	Ahluwalia et al.
3,534,251	A	10/1970	Richards	7,071,692	B2	7/2006	Branch
3,655,178	A	4/1972	Veziha	7,116,198	B1	10/2006	Abele
4,161,172	A	7/1979	Pickering	7,148,689	B2	12/2006	Huang et al.
4,543,959	A	10/1985	Sepponen	7,205,764	B1	4/2007	Anderson et al.
4,567,894	A	2/1986	Bergman	7,255,671	B2	8/2007	Boone
4,612,505	A	9/1986	Zijlstra	7,274,192	B2	9/2007	Havens
4,613,820	A	9/1986	Edelstein	7,278,962	B2	10/2007	Lonneker-Lammers
4,698,611	A	10/1987	Vermilyea	D567,948	S	4/2008	Tierney
4,712,263	A	12/1987	Pronzinski	7,378,848	B2	5/2008	Gao
4,715,073	A	12/1987	Butler	7,400,147	B2	7/2008	Rapoport
4,758,813	A	7/1988	Holsinger et al.	7,423,431	B2	9/2008	Amm et al.
4,875,485	A	10/1989	Matsutani	7,482,558	B2	1/2009	Koch
4,899,109	A	2/1990	Tropp et al.	7,486,982	B2	2/2009	Branch
4,931,733	A	6/1990	Hanawa	7,529,575	B2	5/2009	Rezzonico et al.
4,936,824	A	6/1990	Koch	7,551,954	B2	6/2009	Green et al.
4,968,961	A	11/1990	Miyajima	7,599,728	B2	10/2009	Feenan
5,028,872	A	7/1991	Nakabayashi	7,614,692	B2	11/2009	Biaud
5,038,515	A	8/1991	Moorhead	7,621,815	B2	11/2009	Bosserdet, Jr.
5,059,906	A	10/1991	Yamanaka	7,719,279	B2	5/2010	Rapoport
5,100,375	A	3/1992	Koch	7,777,491	B2	8/2010	Gao
5,153,546	A	10/1992	Laskaris	7,784,121	B2	8/2010	Ahlman
5,235,284	A	8/1993	Tahara et al.	7,800,368	B2	9/2010	Vaughan et al.
5,343,151	A	8/1994	Cory et al.	8,087,203	B2	1/2012	Boesel
5,359,310	A	10/1994	Pissanetzky	8,089,281	B2	1/2012	Zhai et al.
5,436,607	A	7/1995	Chari	8,118,488	B2	2/2012	Gregerson
5,446,934	A	9/1995	Frazier	8,147,396	B2	4/2012	Srinivasan
5,539,316	A	7/1996	Sukumar	8,194,866	B2	6/2012	Smith
5,565,831	A	10/1996	Dorri	8,217,653	B2	7/2012	Vaughan
5,565,834	A	10/1996	Hanley et al.	8,319,496	B2	11/2012	Eryaman et al.
5,635,889	A	6/1997	Stelter	8,390,288	B2	3/2013	Graesslin
5,664,569	A	9/1997	Damadjan et al.	8,405,479	B1	3/2013	Cleveland
5,759,149	A	6/1998	Goldberg	8,525,116	B2	9/2013	Schulz
5,760,585	A	6/1998	Dorri	8,555,578	B2	10/2013	Hushek
5,797,833	A	8/1998	Kobayashi	8,807,084	B2	8/2014	Rapoport
5,800,335	A	9/1998	Koch	8,851,018	B2	10/2014	Rapoport
5,883,558	A	3/1999	Laskaris	8,896,310	B2	11/2014	Rapoport
5,917,324	A	6/1999	Leussler	8,969,829	B2	3/2015	Wollenweber et al.
5,959,454	A	9/1999	Westphal et al.	9,055,912	B2	6/2015	Graumann
5,971,913	A	10/1999	Newkirk	9,100,111	B2	8/2015	Behrendt et al.
6,081,120	A	6/2000	Shen	9,157,975	B2	10/2015	Dale
6,128,522	A	10/2000	Acker	9,159,479	B2	10/2015	Rotem
6,147,578	A	11/2000	Panfil et al.	9,696,269	B2	7/2017	Fordham et al.
6,155,970	A	12/2000	Dykes	9,974,705	B2	5/2018	Rapoport
6,157,278	A	12/2000	Katznelson et al.	10,224,134	B2	3/2019	Nakatsu
6,177,795	B1	1/2001	Zhu et al.	10,224,135	B2*	3/2019	Rapoport ..... H01F 7/0278
6,191,584	B1	2/2001	Trequatrini et al.	2001/0013779	A1	8/2001	Marek
6,208,142	B1	3/2001	Wagshul	2001/0049465	A1	12/2001	Goldberg
6,231,499	B1	5/2001	Jones	2002/0050895	A1	5/2002	Zuk et al.
D446,675	S	8/2001	Straub	2002/0072648	A1	6/2002	Dykes
6,278,274	B1	8/2001	Biglieri	2002/0123681	A1	9/2002	Zuk
6,317,618	B1	11/2001	Livni	2002/0143233	A1	10/2002	Donnelly
6,323,647	B1	11/2001	Anderson	2002/0173717	A1	11/2002	Rohling
6,409,654	B1	6/2002	McClain	2003/0016518	A1	1/2003	Arz
6,411,187	B1	6/2002	Rotem et al.	2003/0088175	A1	5/2003	Branch
6,433,548	B1	8/2002	Furuta	2004/0030241	A1	2/2004	Green
6,452,388	B1	9/2002	Reiderman et al.	2004/0034273	A1	2/2004	Boris
6,471,634	B1	10/2002	Dykes	2004/0106844	A1	6/2004	Lonneker-Lammers
6,511,414	B1	1/2003	Hamsund	2004/0116799	A1	6/2004	Srinivasan
6,535,092	B1	3/2003	Hurley et al.	2004/0127786	A1	7/2004	Schmit
6,600,401	B2	7/2003	Zuk et al.	2004/0133064	A1	7/2004	Castillon Levano
6,611,702	B2	8/2003	Rohling	2004/0135687	A1	7/2004	Keene
6,641,521	B2	11/2003	Kolarovic	2004/0147833	A1	7/2004	Czipott
6,646,530	B2	11/2003	Ruhrig	2004/0186341	A1	9/2004	McDermott
6,666,816	B2	12/2003	Mountain	2004/0194989	A1	10/2004	Branch
6,687,526	B2	2/2004	Brand et al.	2004/0196043	A1	10/2004	Branch
RE38,453	E	3/2004	Lessard	2005/0020906	A1	1/2005	Seijger
6,707,363	B1	3/2004	Abele	2005/0027189	A1	2/2005	Branch
6,751,496	B2	6/2004	Su et al.	2005/0030028	A1	2/2005	Clarke et al.
6,776,527	B1	8/2004	Tybinkowski	2005/0038314	A1	2/2005	Falk
6,838,964	B1	1/2005	Knight et al.	2005/0043612	A1	2/2005	Saint-Jalmes et al.
6,860,272	B2	3/2005	Carter	2005/0113668	A1	5/2005	Srinivasan
6,897,750	B2	5/2005	Neuberth	2006/0267585	A1	11/2006	Havens
				2007/0068862	A1	3/2007	Sisemore
				2007/0096737	A1	5/2007	Rapoport
				2007/0108850	A1	5/2007	Chertok
				2007/0135704	A1	6/2007	Branch

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2007/0232894 A1 10/2007 Feenan  
 2007/0238950 A1 10/2007 Vija  
 2007/0249928 A1 10/2007 Blezek et al.  
 2007/0265520 A1 11/2007 Posse  
 2007/0273378 A1 11/2007 Trequattrini et al.  
 2008/0001601 A1 1/2008 Sellers et al.  
 2008/0103388 A1 5/2008 Maschke  
 2008/0122441 A1 5/2008 Hayakawa  
 2008/0163425 A1 7/2008 White  
 2008/0171931 A1 7/2008 Maschke  
 2008/0204028 A1 8/2008 Devries  
 2008/0234571 A1 9/2008 Hay  
 2008/0246476 A1 10/2008 Rapoport  
 2008/0259560 A1 10/2008 Lvovsky  
 2008/0281187 A1 11/2008 Massengill  
 2009/0072939 A1 3/2009 Shen et al.  
 2009/0085700 A1 4/2009 Lian et al.  
 2009/0120615 A1 5/2009 Icoz et al.  
 2009/0209846 A1 8/2009 Bammer  
 2009/0237077 A1 9/2009 Vaughan  
 2010/0004502 A1 1/2010 Honma  
 2010/0066368 A1 3/2010 Gao  
 2010/0145358 A1 6/2010 Maschke  
 2010/0154325 A1 6/2010 Boesel  
 2010/0168502 A1 7/2010 Delaporte  
 2010/0172468 A1 7/2010 Gregerson  
 2010/0198047 A1 8/2010 Zagorchev  
 2010/0219347 A1 9/2010 Schulz  
 2010/0245543 A1 9/2010 Greer  
 2010/0315085 A1 12/2010 Brown  
 2011/0048424 A1 3/2011 Radko  
 2011/0090033 A1 4/2011 Sankar  
 2011/0113555 A1 5/2011 Smith  
 2011/0125010 A1 5/2011 Vaquero Lopez  
 2011/0162652 A1 7/2011 Rapoport  
 2011/0274238 A1 11/2011 Maschke  
 2011/0280364 A1 11/2011 Maschke  
 2011/0280380 A1 11/2011 Maschke  
 2011/0282184 A1 11/2011 Klingenbeck  
 2011/0304333 A1 12/2011 Rapoport  
 2012/0071745 A1 3/2012 Rapoport  
 2012/0073511 A1 3/2012 Rapoport  
 2012/0077707 A1 3/2012 Rapoport  
 2012/0078034 A1 3/2012 Falk  
 2012/0119742 A1 5/2012 Rapoport  
 2012/0126814 A1 5/2012 Fischer  
 2012/0140899 A1 6/2012 Bailey  
 2013/0079624 A1 3/2013 Rapoport  
 2013/0109956 A1 5/2013 Rapoport  
 2013/0204074 A1 8/2013 Belval  
 2013/0204617 A1 8/2013 Kuo  
 2013/0267765 A1 10/2013 Rapoport  
 2013/0328560 A1 12/2013 Rapoport  
 2014/0003614 A1 1/2014 Levitov  
 2014/0051976 A1 2/2014 Rapoport  
 2014/0055136 A1 2/2014 Leussler  
 2014/0078301 A1 3/2014 Fazzi  
 2014/0099010 A1 4/2014 Rapoport  
 2014/0117989 A1 5/2014 Rapoport  
 2014/0128725 A1 5/2014 Rapoport  
 2014/0139216 A1 5/2014 Rapoport  
 2014/0152302 A1 6/2014 Rapoport  
 2014/0152310 A1 6/2014 Rapoport  
 2014/0158062 A1 6/2014 Rapoport  
 2014/0230850 A1 8/2014 Rapoport  
 2014/0257081 A1 9/2014 Rapoport  
 2014/0266203 A1 9/2014 Rapoport  
 2014/0300358 A1 10/2014 Rapoport  
 2014/0354279 A1 12/2014 Dumoulin  
 2014/0357981 A1 12/2014 Dumoulin  
 2014/0364722 A1 12/2014 Dumoulin  
 2014/0378821 A1 12/2014 Rapoport  
 2014/0378825 A1 12/2014 Rapoport  
 2015/0005618 A1 1/2015 Dumoulin  
 2015/0059157 A1 3/2015 Rapoport

2015/0059655 A1 3/2015 Rapoport  
 2015/0061680 A1 3/2015 Leskowitz  
 2015/0065788 A1 3/2015 Rapoport  
 2015/0077105 A1 3/2015 Rapoport  
 2015/0137812 A1 5/2015 Rapoport  
 2015/0141799 A1 5/2015 Rapoport  
 2015/0168519 A1 6/2015 Rapoport  
 2015/0226817 A1 8/2015 Pourrahimi  
 2015/0230766 A1 8/2015 Wang  
 2015/0253397 A1 9/2015 Rapoport  
 2015/0253400 A1 9/2015 Rapoport  
 2015/0253401 A1 9/2015 Rapoport  
 2016/0022123 A1 1/2016 Katznelson et al.  
 2016/0030264 A1 2/2016 Lehmann  
 2016/0032712 A1 2/2016 Frosell et al.  
 2016/0081582 A1 3/2016 Rapoport  
 2016/0089054 A1 3/2016 Rapoport  
 2017/0143271 A1 5/2017 Gustafsson  
 2017/0146619 A1 5/2017 Strauss  
 2017/0181912 A1 6/2017 Rapoport  
 2019/0170840 A1 6/2019 Rapoport  
 2019/0172620 A1 6/2019 Rapoport

## FOREIGN PATENT DOCUMENTS

CN 2448344 9/2001  
 CN 101185383 5/2008  
 CN 201846566 5/2011  
 CN 102136337 7/2011  
 CN 102551719 A 7/2012  
 CN 103565437 B 2/2014  
 CN 104207773 A 12/2014  
 DE 19617739 6/1997  
 DE 102008009673 8/2009  
 DE 102008009674 8/2009  
 EP 0187691 7/1986  
 EP 0921527 6/1999  
 EP 0921537 6/1999  
 EP 1619667 1/2006  
 EP 2581071 4/2013  
 EP 2607977 6/2013  
 GB 863272 3/1961  
 IL 226488 7/2016  
 JP S5961763 4/1984  
 JP H04317630 11/1992  
 JP 2004531313 10/2004  
 JP 2005514078 5/2005  
 JP 2007252741 10/2007  
 JP 2010178857 8/2010  
 WO 8910722 A1 11/1989  
 WO 9848756 A1 11/1998  
 WO 9921526 5/1999  
 WO 2004029644 4/2004  
 WO WO2005074608 8/2005  
 WO WO2007/052275 5/2007  
 WO 2010125559 11/2010  
 WO WO2011/001429 1/2011  
 WO 2011109761 9/2011  
 WO 2012004797 1/2012  
 WO 2012143825 A1 10/2012  
 WO 2013115847 8/2013  
 WO WO2014/141251 9/2014  
 WO 2014188424 11/2014  
 WO 2014188426 11/2014  
 WO 2018029666 2/2018

## OTHER PUBLICATIONS

Yingying Yao, Yong-Kwon Choi and Chang-Seop Koh, The Optimal Design of Passive Shimming Elements for High Homogenous Permanent Magnets Utilizing Sensitivity Analysis, Journal of Electrical Engineering & Technology, 2006, vol. I, No. 4, pp. 461-465.  
 Z. Ren, D. Xie, and H. Li, Study on Shimming Method for Open Permanent Magnet of MRI, Progress in Electromagnetics Research M, 2009, vol. 6, 23-34.  
 Keith Wachowicz, Evaluation of Active and Passive Shimming in Magnetic Resonance Imaging, Research and Reports in Nuclear Medicine, 2014:4 1-12.

(56)

**References Cited**

## OTHER PUBLICATIONS

R Prost and L F Czervionke, How does an MR scanner operate? American Journal of Neuroradiology, Aug. 1994, 15 (7) 1383-1386.

Belov, A. et al. Passive Shimming of the Superconducting Magnet for MRI, IEEE Transactions on Applied Superconductivity, Jun. 1995, vol. 5, No. 2, 679-681.

McGinley et al., A permanent MRI magnet for magic angle imaging having its field parallel to the poles, Journal of Magnetic Resonance, 2016, 271; 60-67.

Advanced Healthcare Technology, "Baby Pod II: Infant Transport Device", pp. 1-6, accessed online on May 26, 2016.

Advanced Healthcare Technology, "Baby Pod II: Operating & Maintenance Manual", revised Jan. 2011, pp. 1-14.

Aspect Imaging Ltd., "MRI-Incubator's Closure Assembly", co-pending U.S. Appl. No. 14/539,442, filed Nov. 12, 2014.

Aspect Imaging Ltd., "MRI RF Shielding Jacket", co-pending U.S. Appl. No. 14/623,051, filed Feb. 16, 2015.

Aspect Imaging Ltd., "MRI Thermo-Isolating Jacket", co-pending U.S. Appl. No. 14/623,039, filed Feb. 16, 2015.

Aspect Imaging Ltd., "A Method for Providing High Resolution, High Contrast Fused MRI Images", co-pending U.S. Appl. No. 13/877,553, filed Apr. 3, 2013.

Aspect Imaging Ltd., "Cage in an MRD with a Fastening/Attenuating System", co-pending U.S. Appl. No. 14/527,950, filed Oct. 30, 2014.

Aspect Imaging Ltd., "Foamed Patient Transport Incubator", co-pending U.S. Appl. No. 14/531,289, filed Nov. 3, 2014.

Aspect Imaging Ltd., "Incubator Deployable Multi-Functional Panel", co-pending U.S. Appl. No. 14/619,557, filed Feb. 11, 2015.

Aspect Imaging Ltd., "Incubator's Canopy with Sensor Dependent Variably Transparent Walls and Methods for Dimming Lights Thereof", co-pending U.S. Appl. No. 14/453,909, filed Aug. 7, 2014.

Aspect Imaging Ltd., "Means and Method for Operating an MRI Device Within a RF-Magnetic Environment", copending U.S. Appl. No. 14/596,329, filed Jan. 14, 2015.

Aspect Imaging Ltd., "Means for Operating an MRI Device Within a RF-Magnetic Environment", co-pending U.S. Appl. No. 14/596,320, filed Jan. 14, 2015.

Aspect Imaging Ltd., "Mechanical Clutch for MRI", co-pending U.S. Appl. No. 14/611,379, filed Feb. 2, 2015.

Aspect Imaging Ltd., "Shutting Assembly for Closing an Entrance of an MRI Device", co-pending U.S. Appl. No. 14/540,163, filed Nov. 13, 2014.

Aspect Imaging Ltd., "Method for Providing High Resolution, High Contrast Fused MRI Images", co-pending U.S. Appl. No. 13/877,553, filed Apr. 3, 2013.

Eberich et al., Functional MRI in neonates using neonatal head coil and MR compatible incubator, NeuroImage 20 (2003) 683-692.

International Preliminary Report on Patentability for PCT Application No. PCT/IL2014/50450 dated May 8, 2015.

International Search Report dated Jul. 27, 2012 in corresponding International Application No. PCT/IL2011/000537.

International Search Report for Application No. EP17785567.3, dated Nov. 20, 2019, 7 pages.

International Search Report for PCT Application No. PCT/IL2014/50451 dated Mar. 16, 2015.

International Search Report from PCT/IL2014/050450, dated May 21, 2014.

Jenkins, S., ScanPod, Baby Pod-Products-Scan Pod, 2002-2011 Advance Healthcare Technology, Ltd., internet website <http://babypod.com:80/products/scanpod.php>.

Office Action dated Jan. 15, 2020 for U.S. Appl. No. 16/040,214 (6 pages).

Office Action for U.S. Appl. No. 14/892,209 dated Sep. 28, 2016.

Paley et al., An MR-compatible neonatal incubator, The British Journal of Radiology, 85, 2012, 952-958.

Rapoport, URI, "RF Shielding Conduit in an MRI Closure Assembly", co-pending U.S. Appl. No. 14/574,785, filed Dec. 18, 2014.

Science Daily, Inside the preemie brain, Incubator enables MRI scans on preemies for preventing birth asphyxia, Dec. 1, 2005, pp. 1-2, Web address: [http://web.archive.org/web/20130303154220/http://www.sciencedaily.com/videos/2005/1211-inside\\_the\\_preemie\\_brain.htm](http://web.archive.org/web/20130303154220/http://www.sciencedaily.com/videos/2005/1211-inside_the_preemie_brain.htm).

Science Museum, "Fast Forward: 20 ways F1 is changing our world-Baby Pod II", uploaded Apr. 7, 2009, accessed online on May 26, 2016 at <https://www.youtube.com/watch?v=KyZVhPWbWqo>.

U.S. Appl. No. 61/899,233, filed Nov. 3, 2013 Rapoport.

U.S. Appl. No. 61/940,514, filed Feb. 17, 2014 Rapoport.

U.S. Appl. No. 61/905,221, filed Nov. 17, 2013 Rapoport.

Canadian Examiner Requisition for Application No. CA3,033,328, dated Jan. 31, 2020, 3 pages.

\* cited by examiner

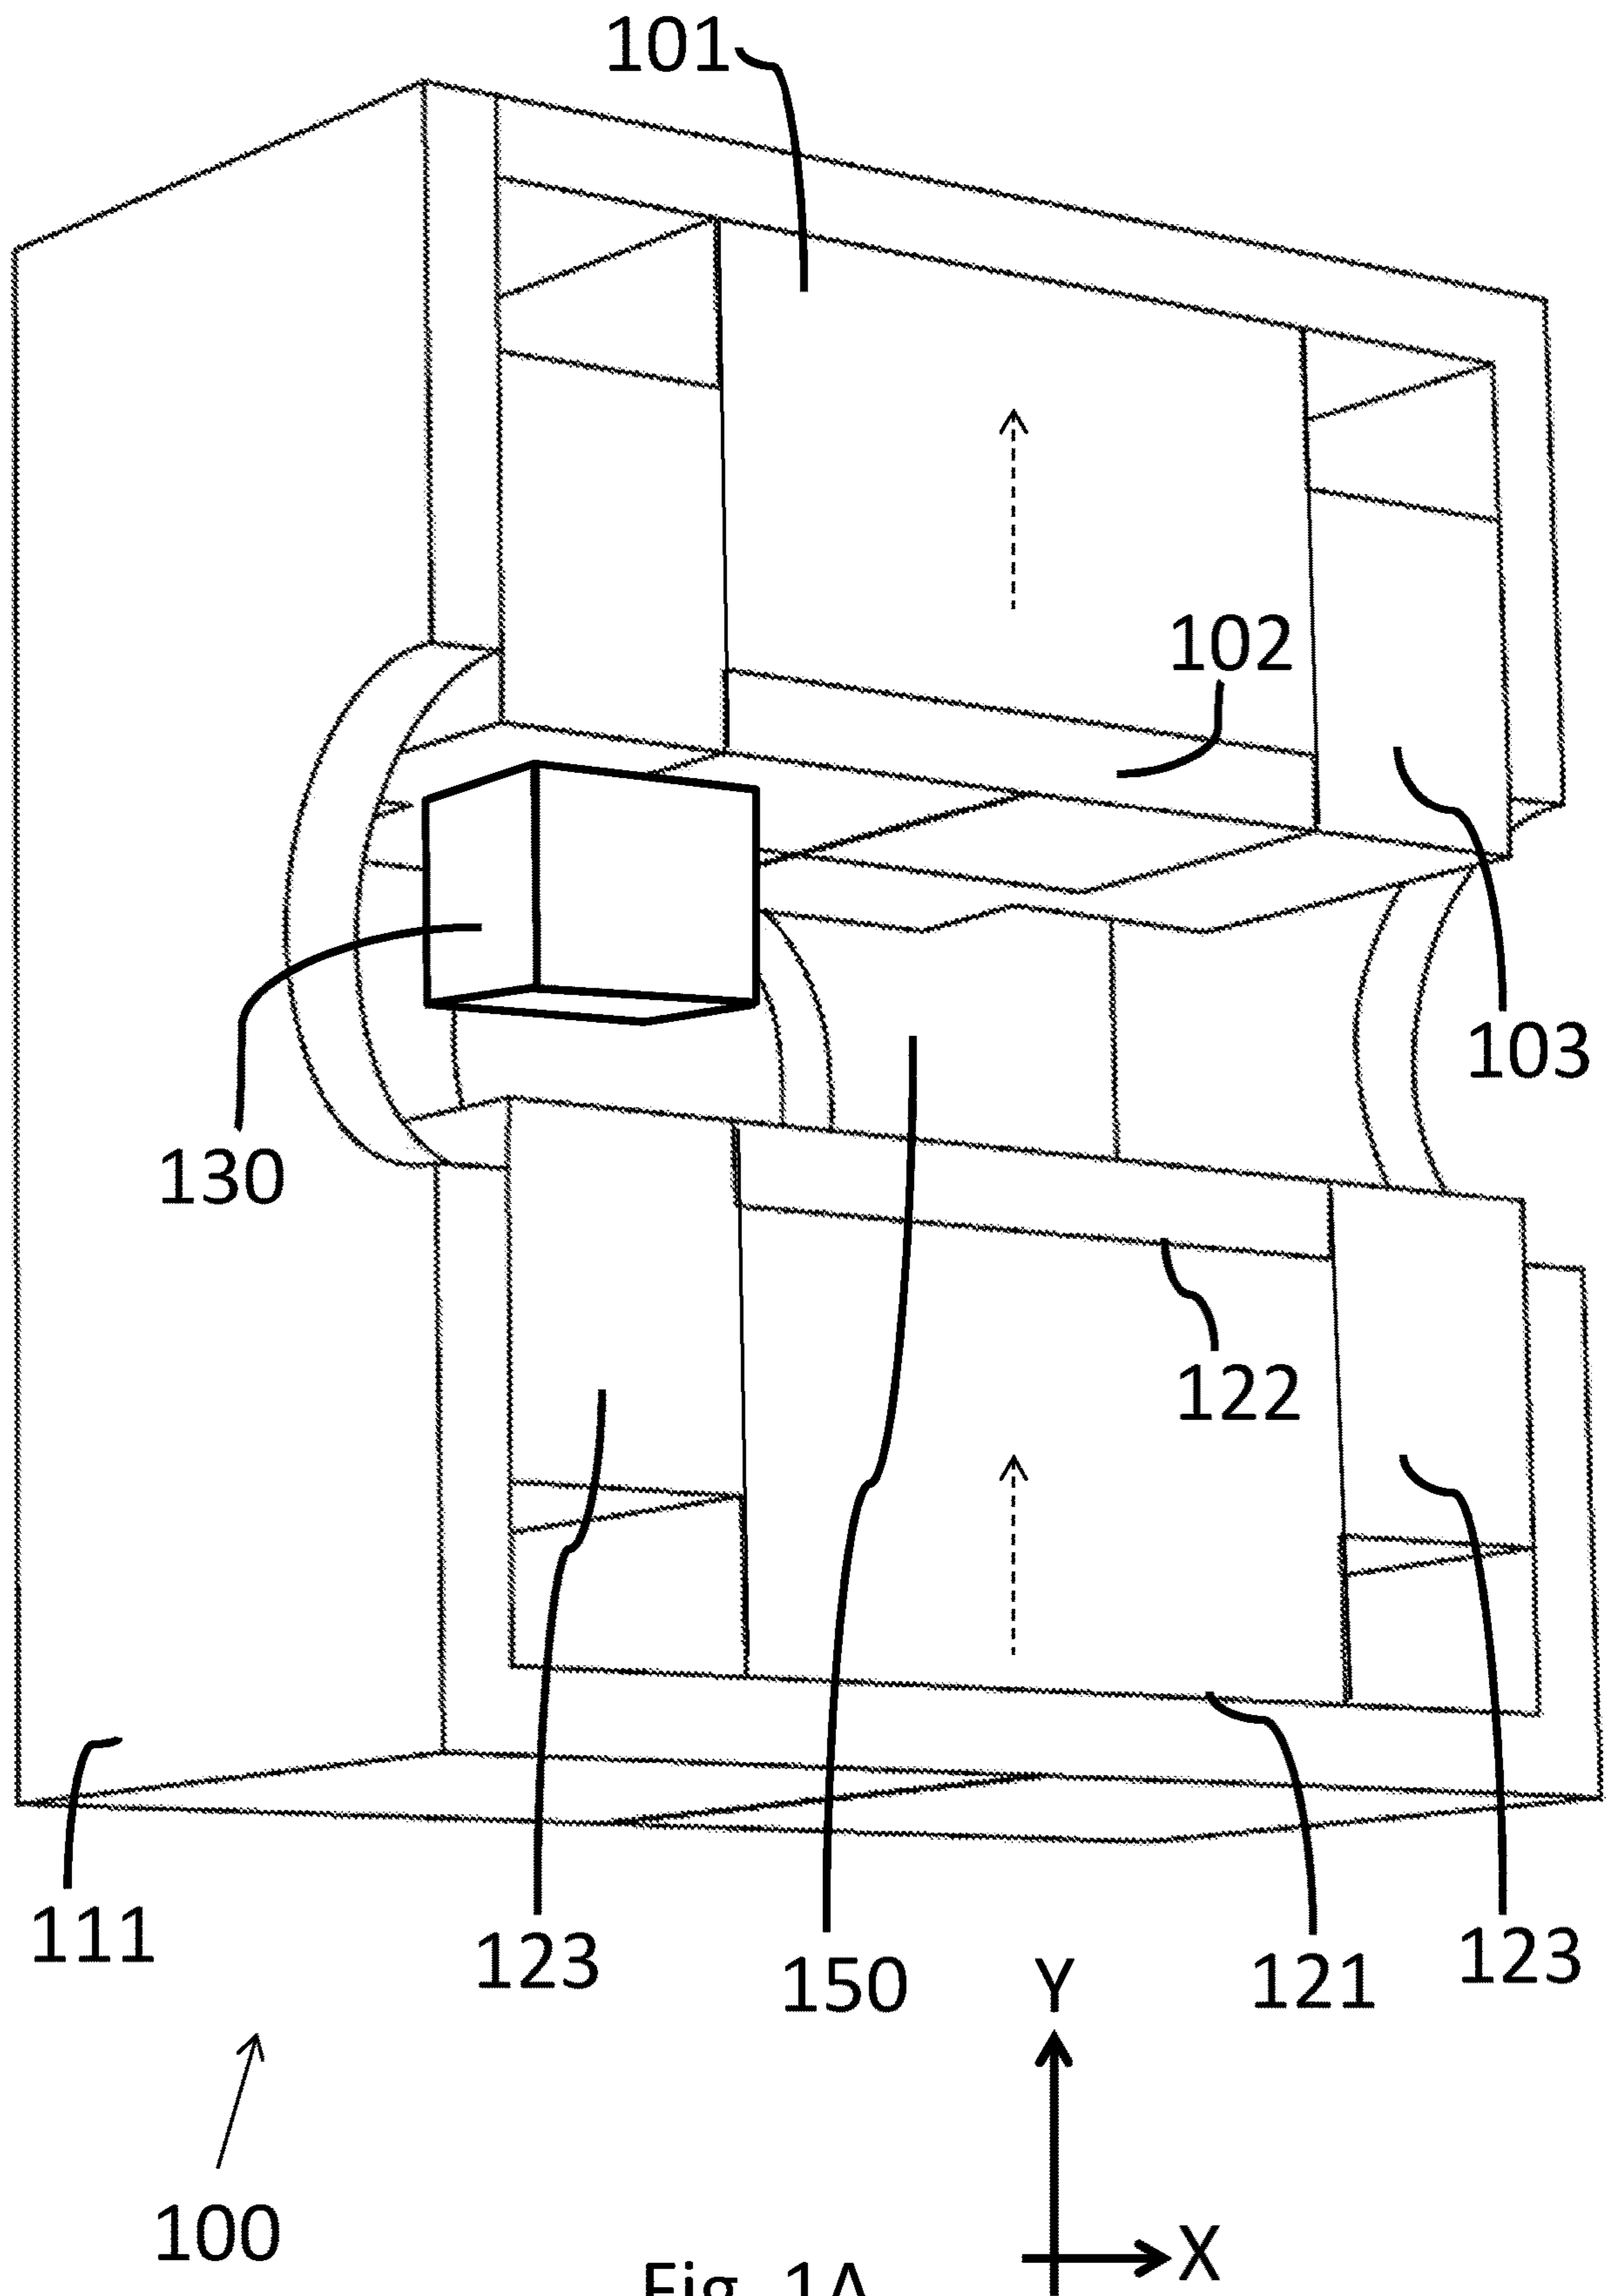


Fig. 1A

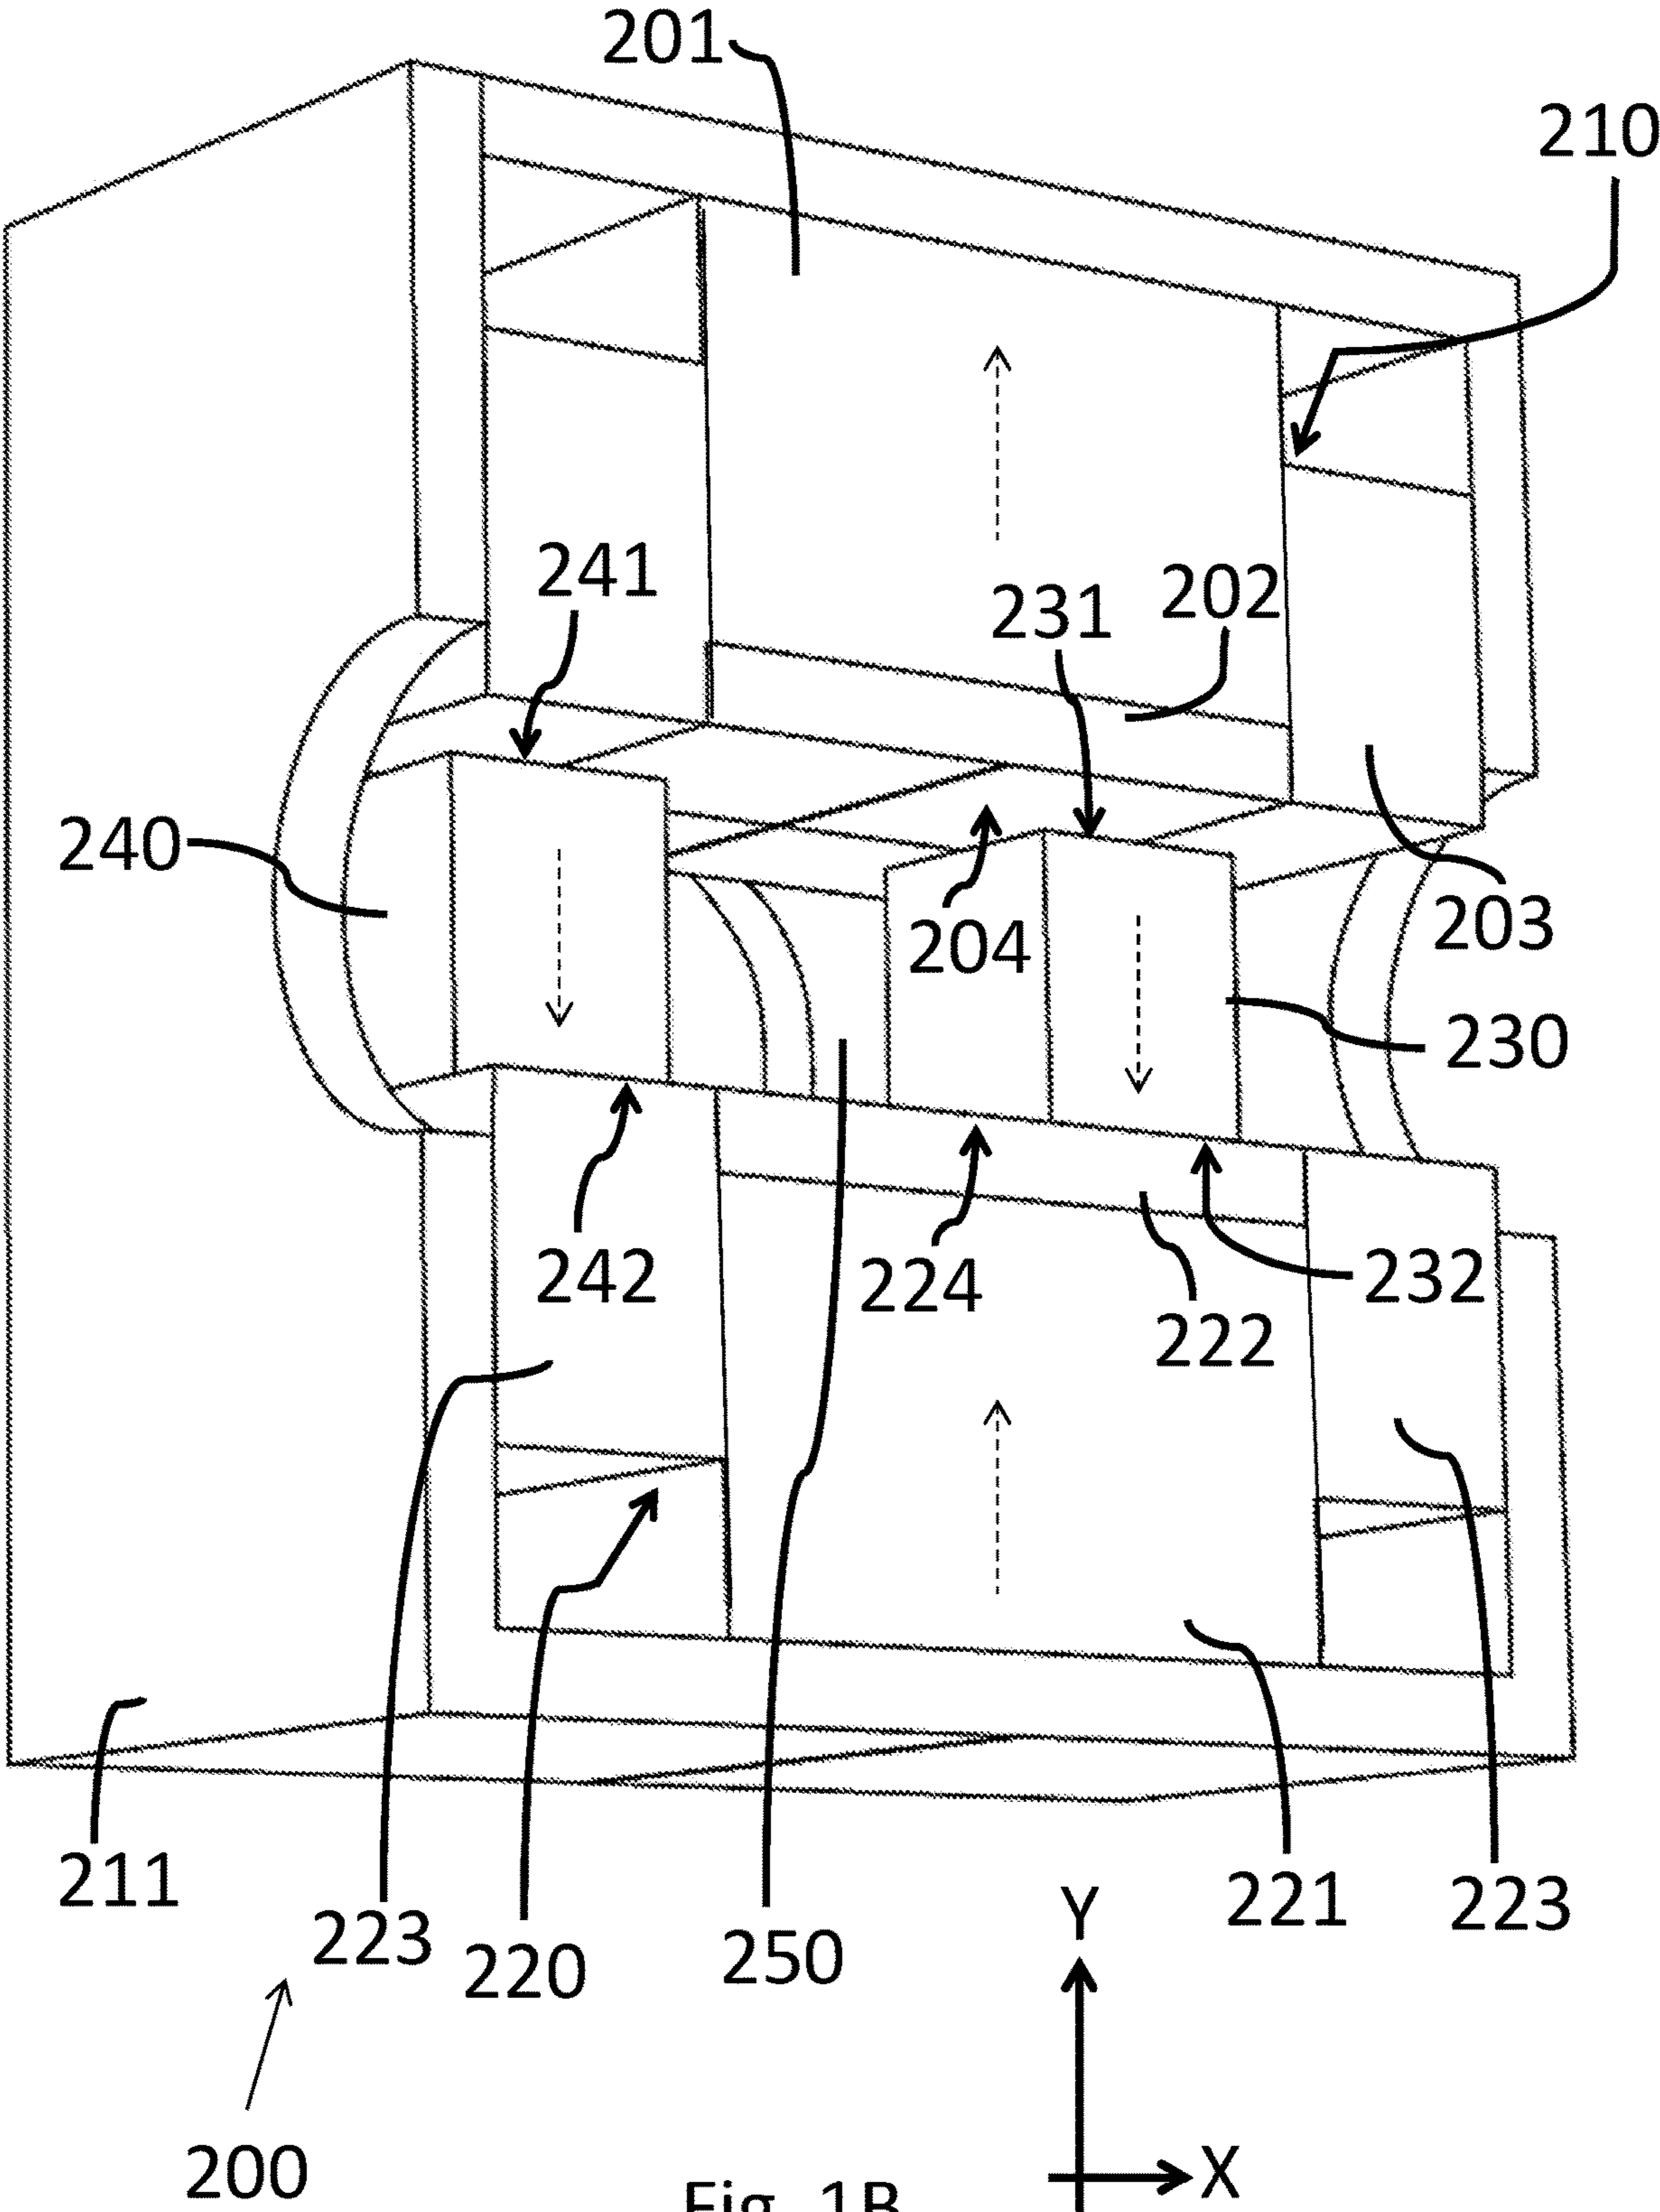


Fig. 1B

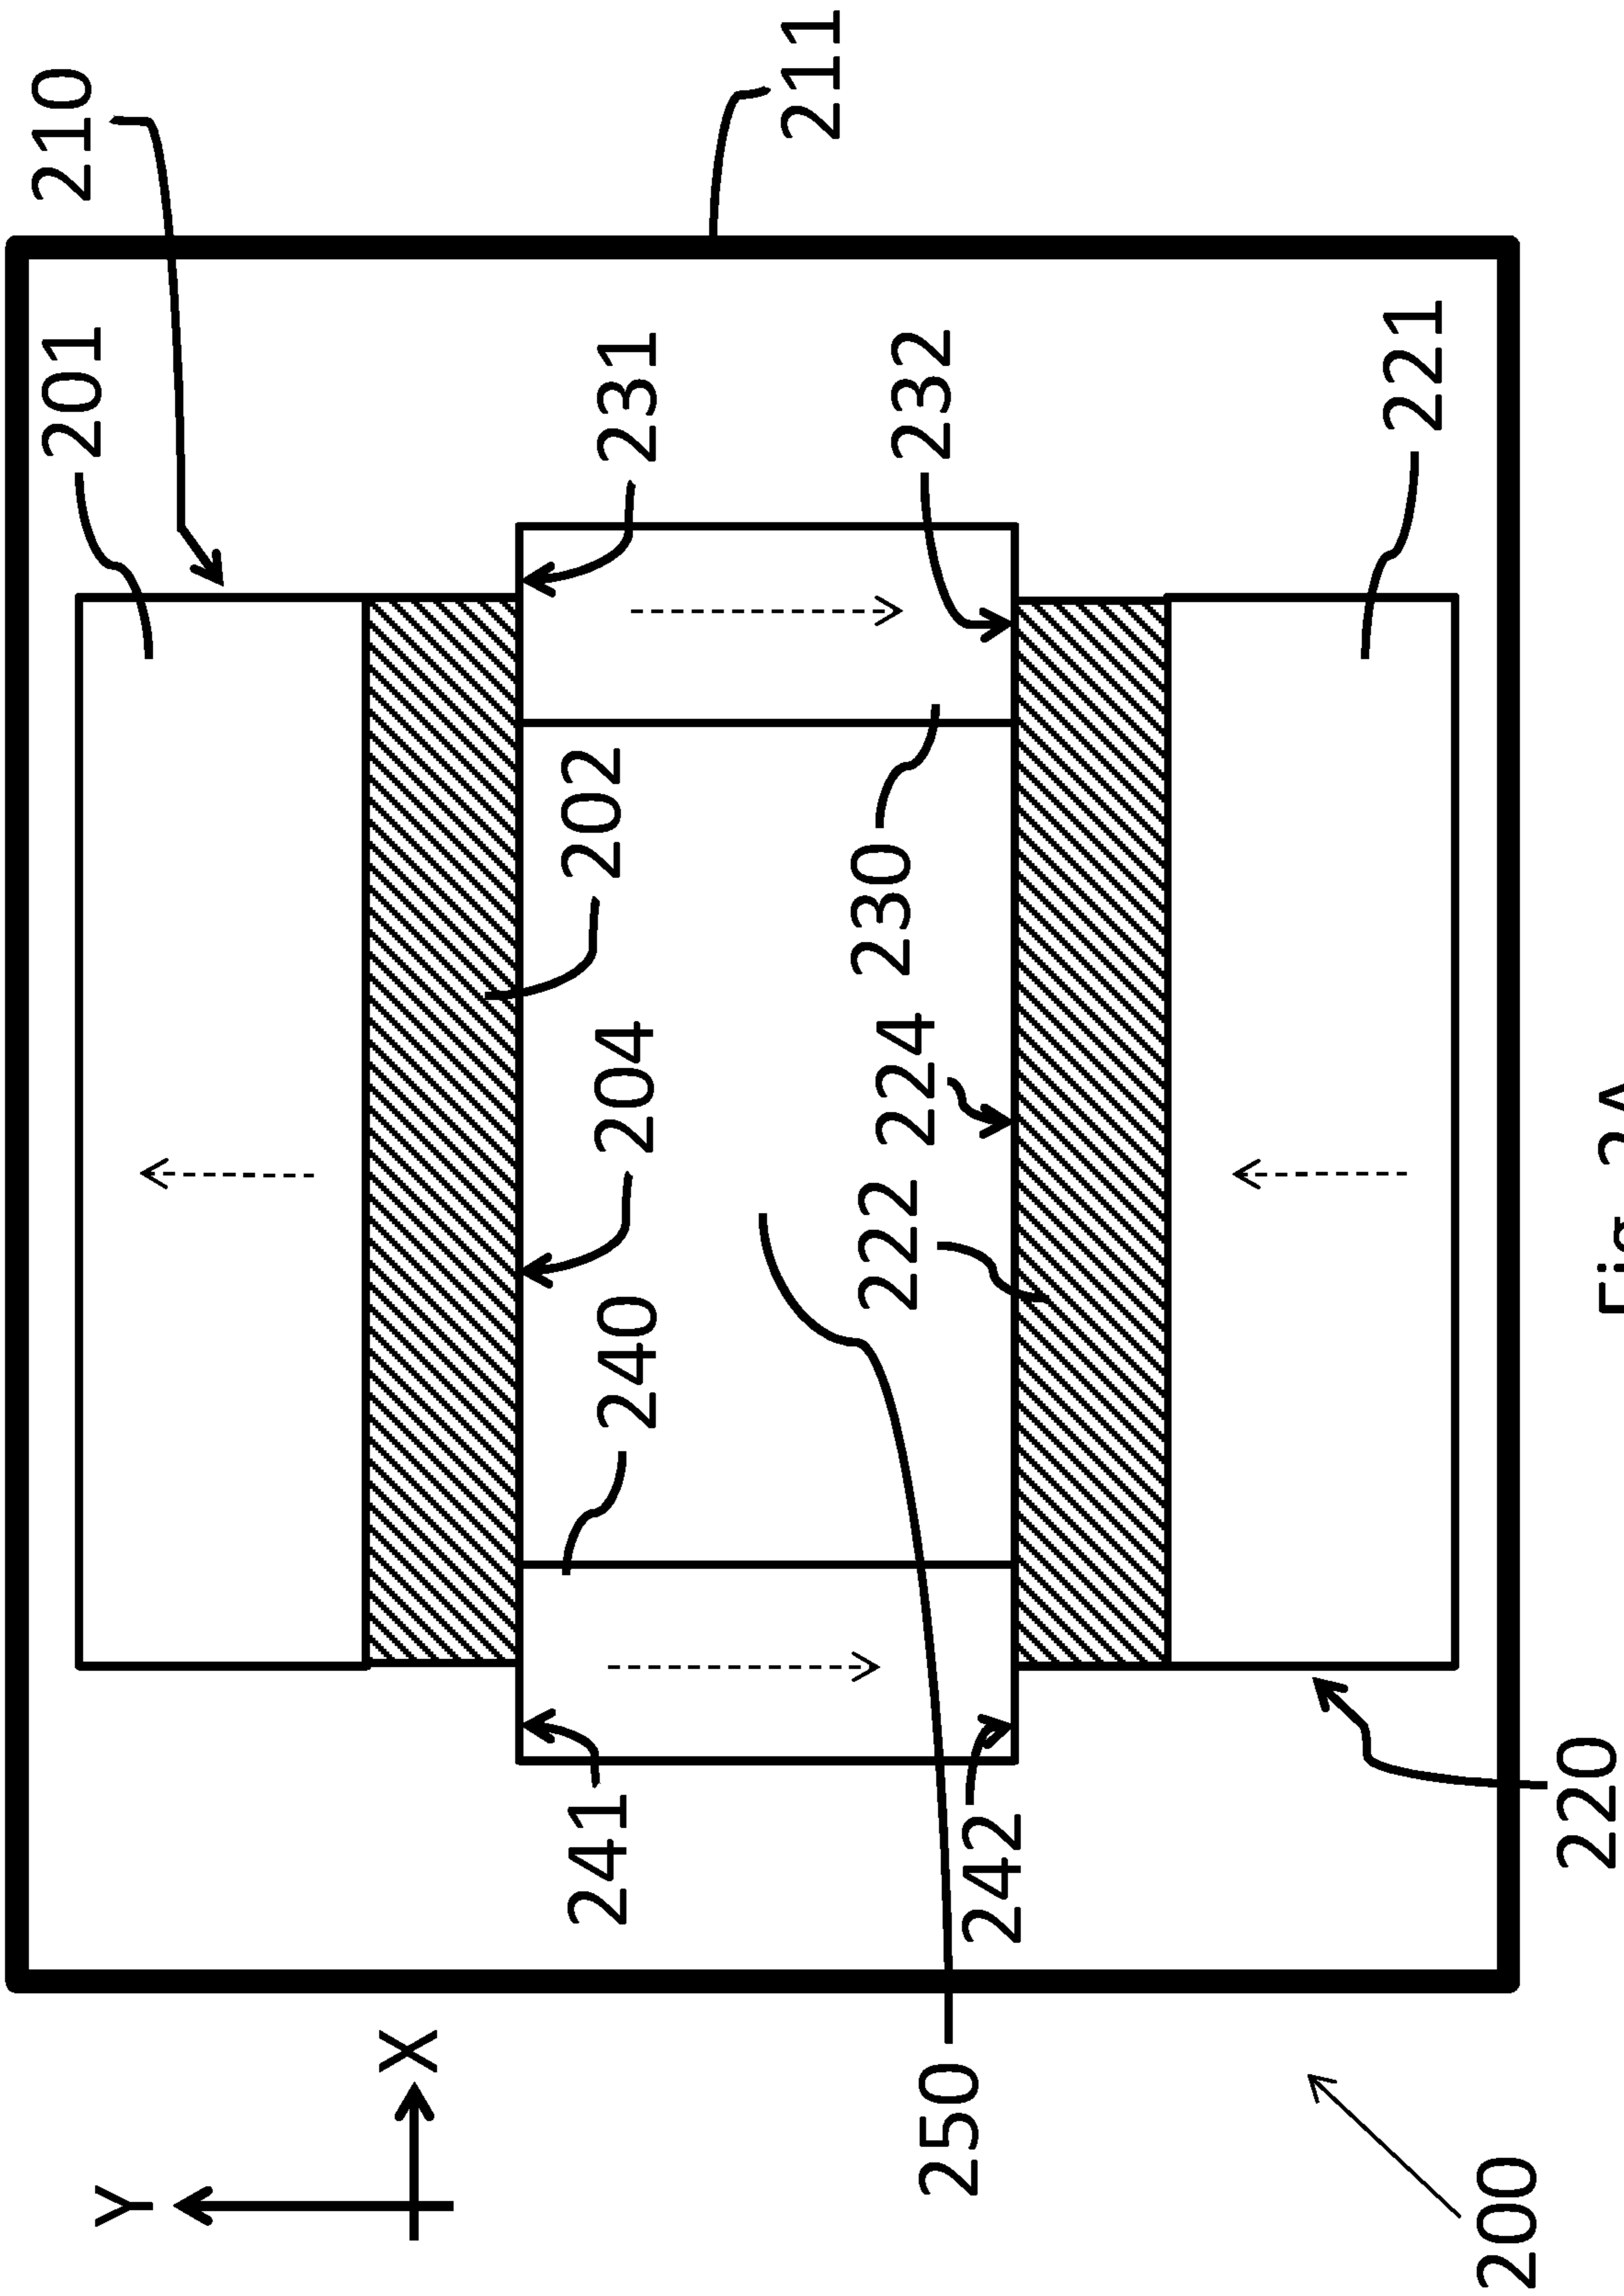


Fig. 2A

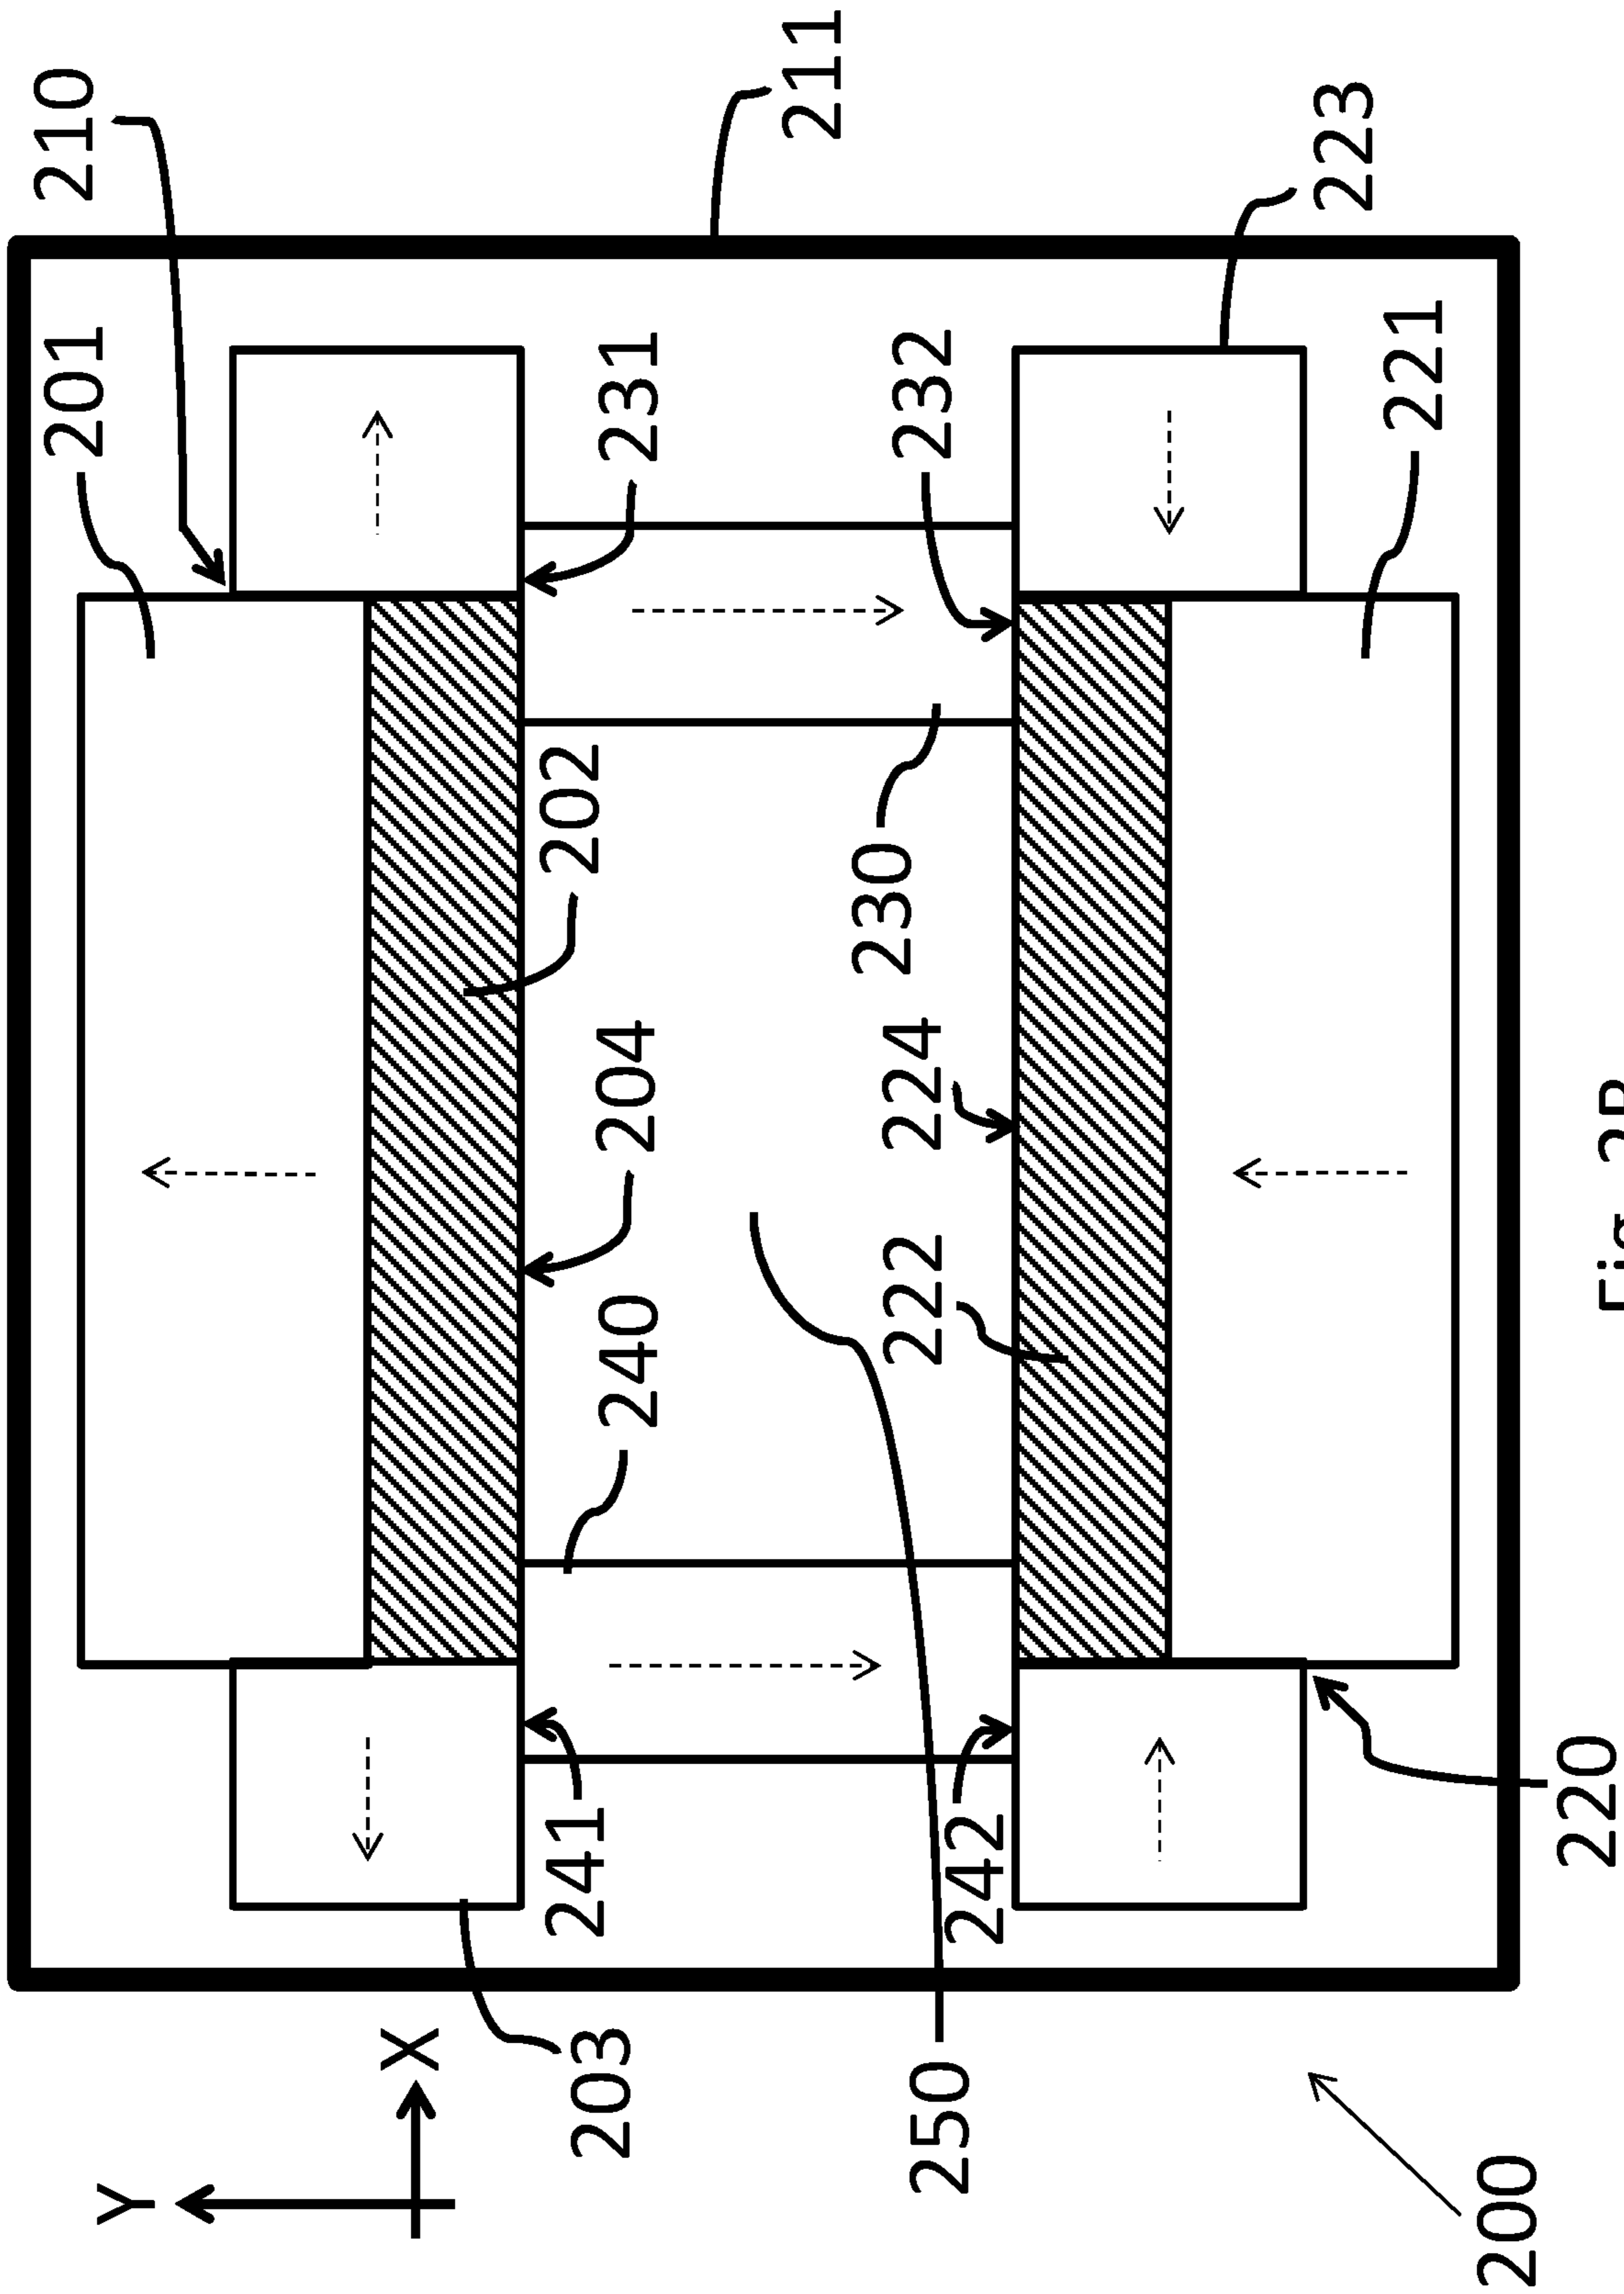


Fig. 2B



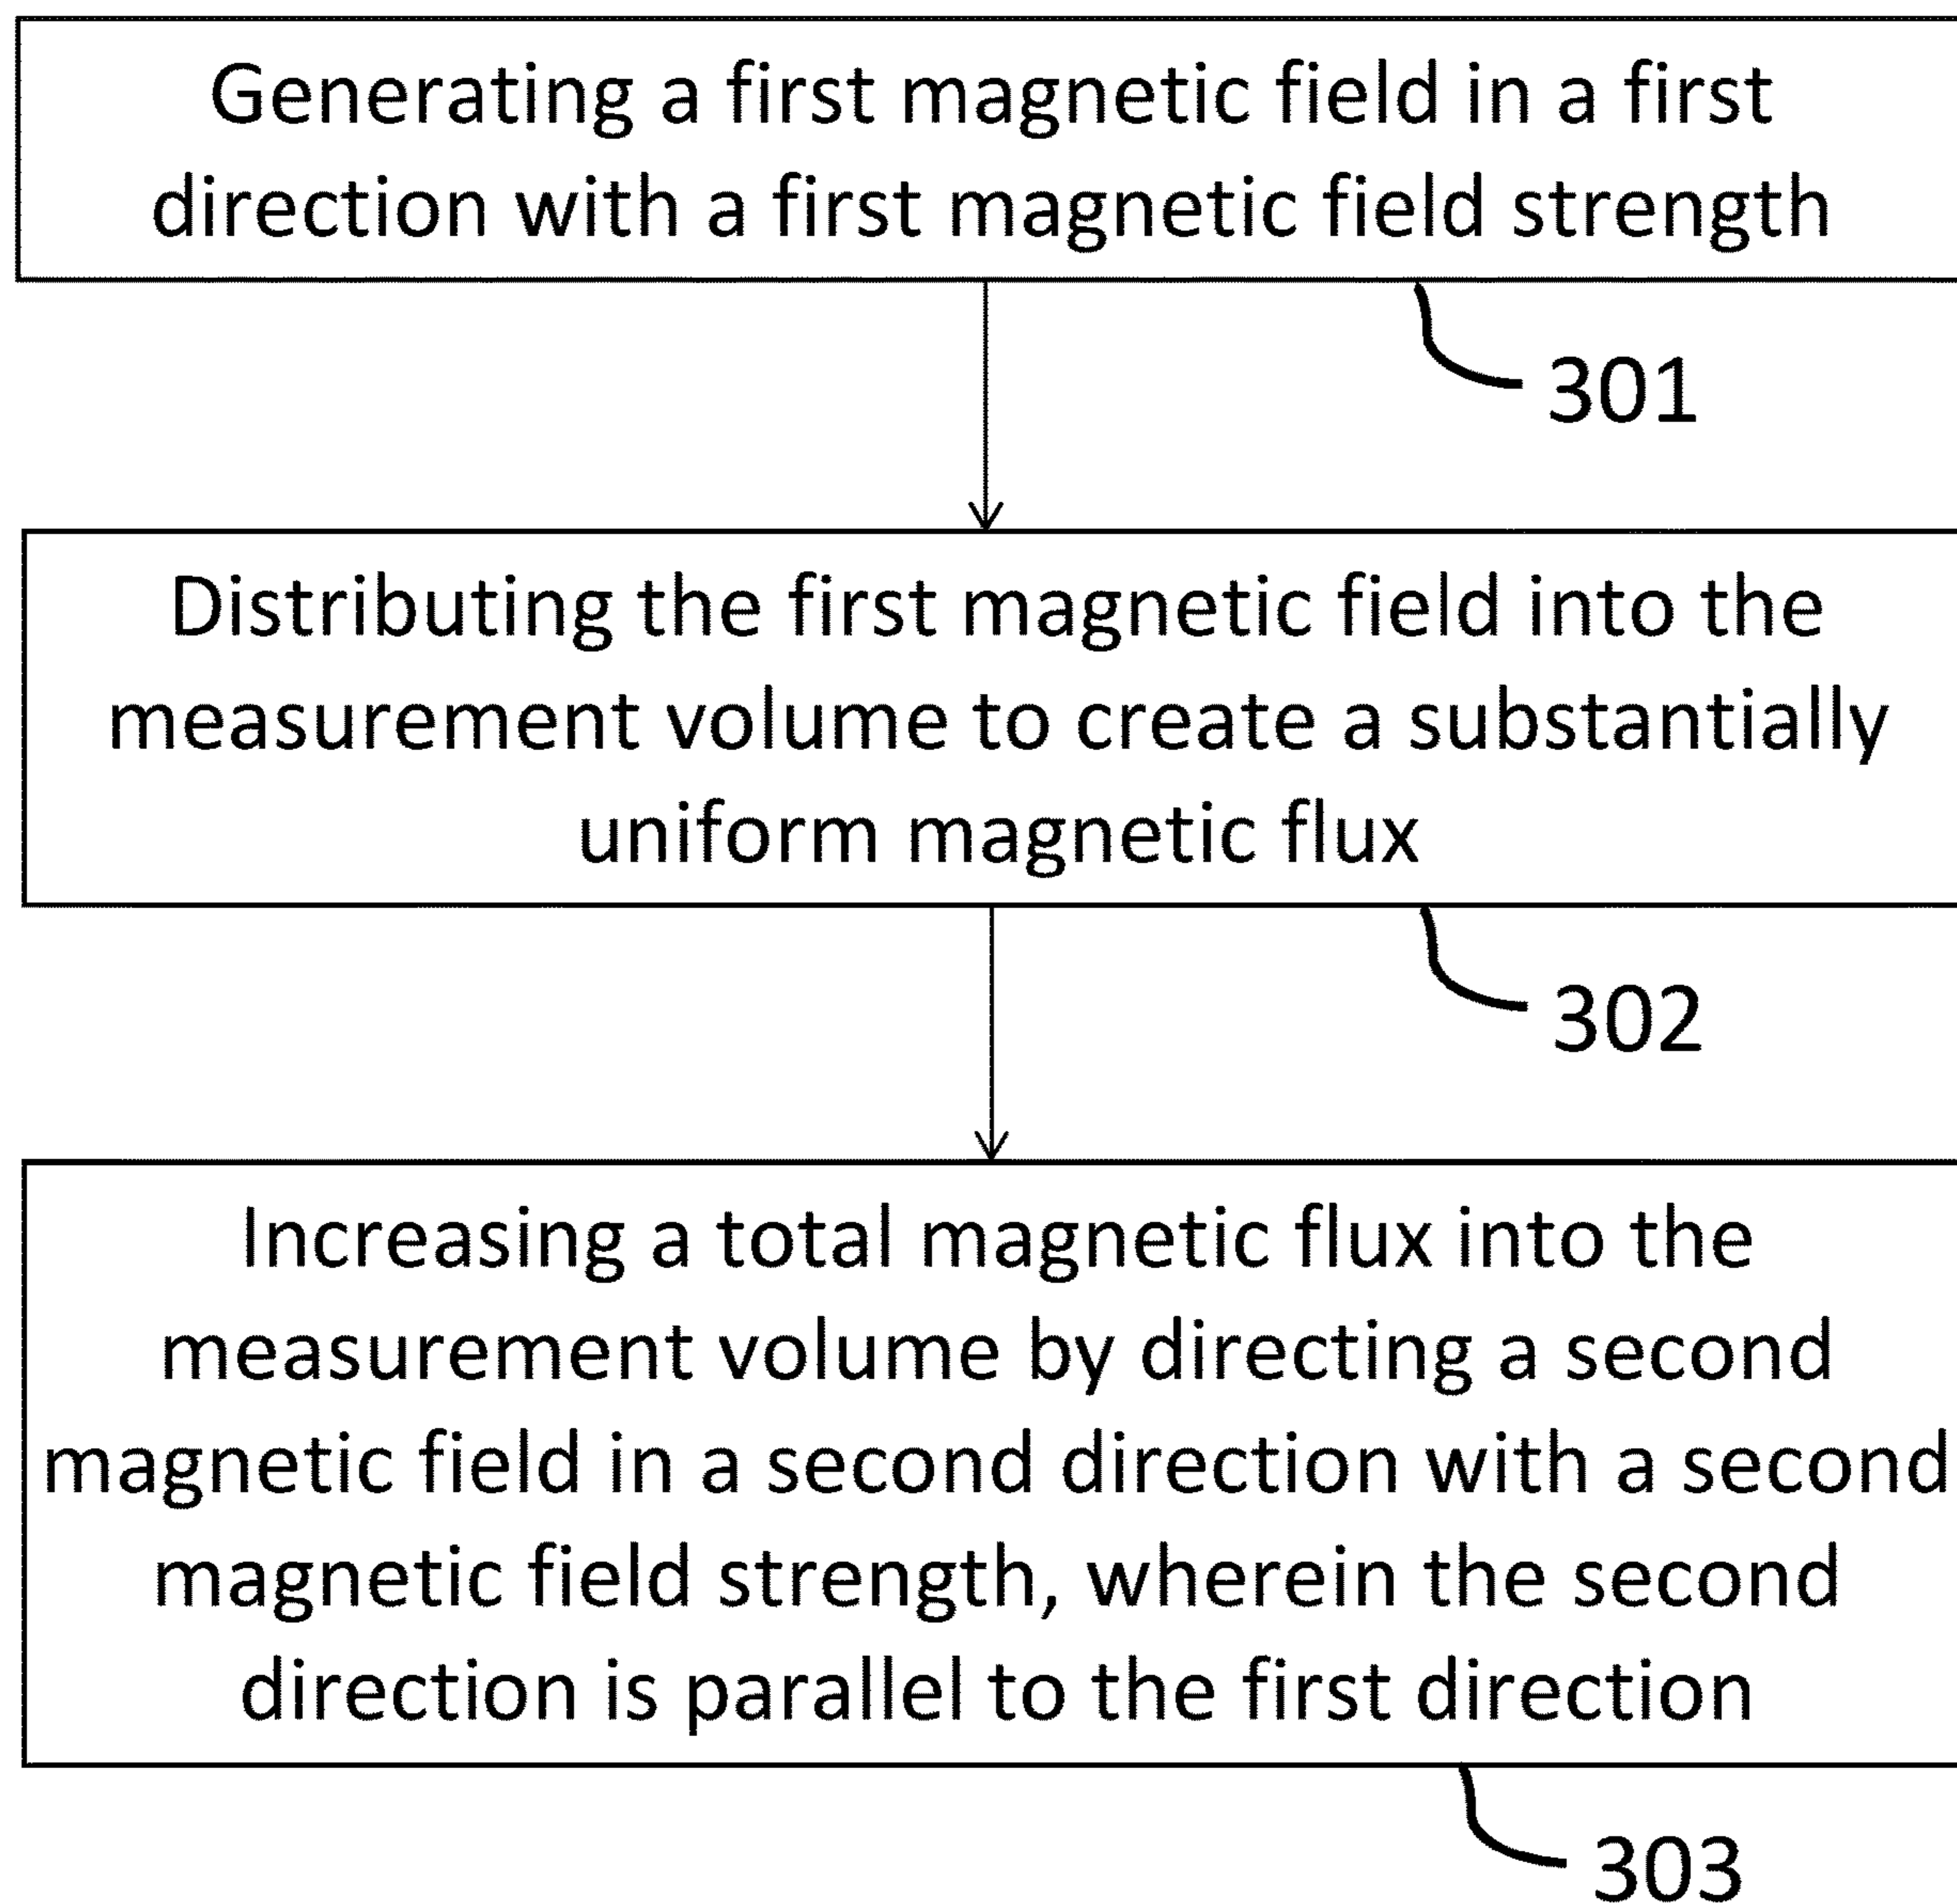
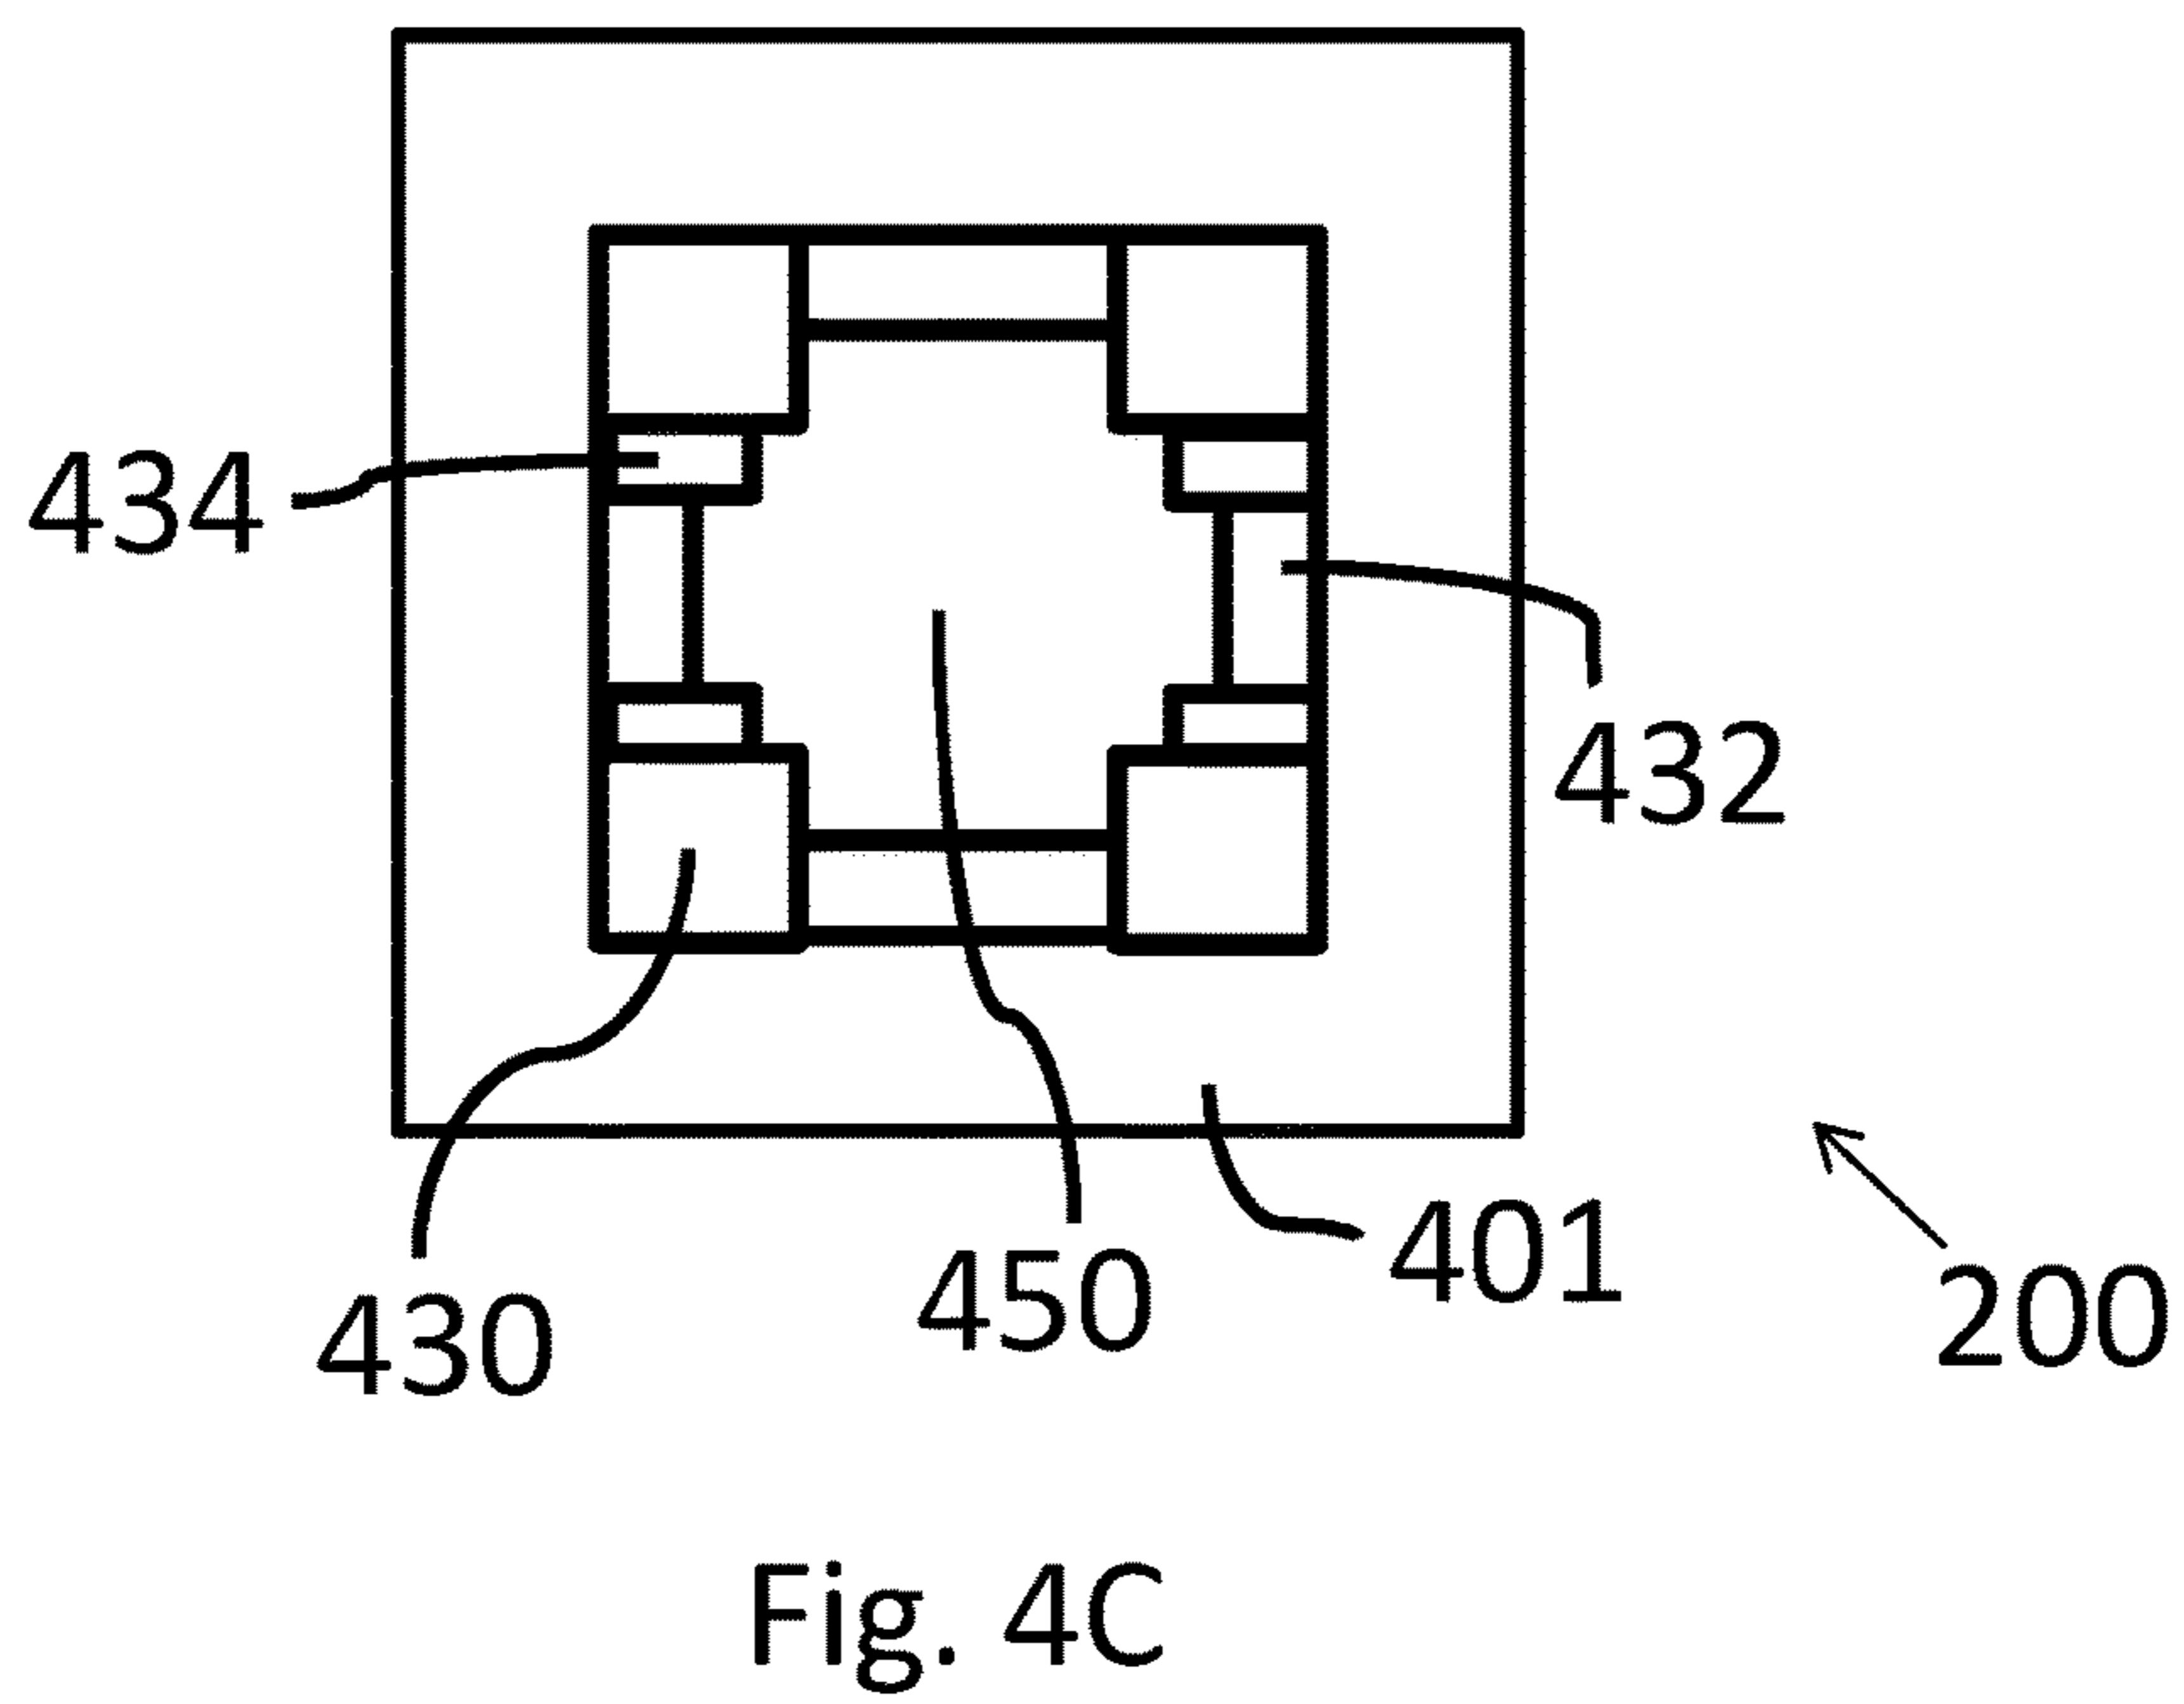
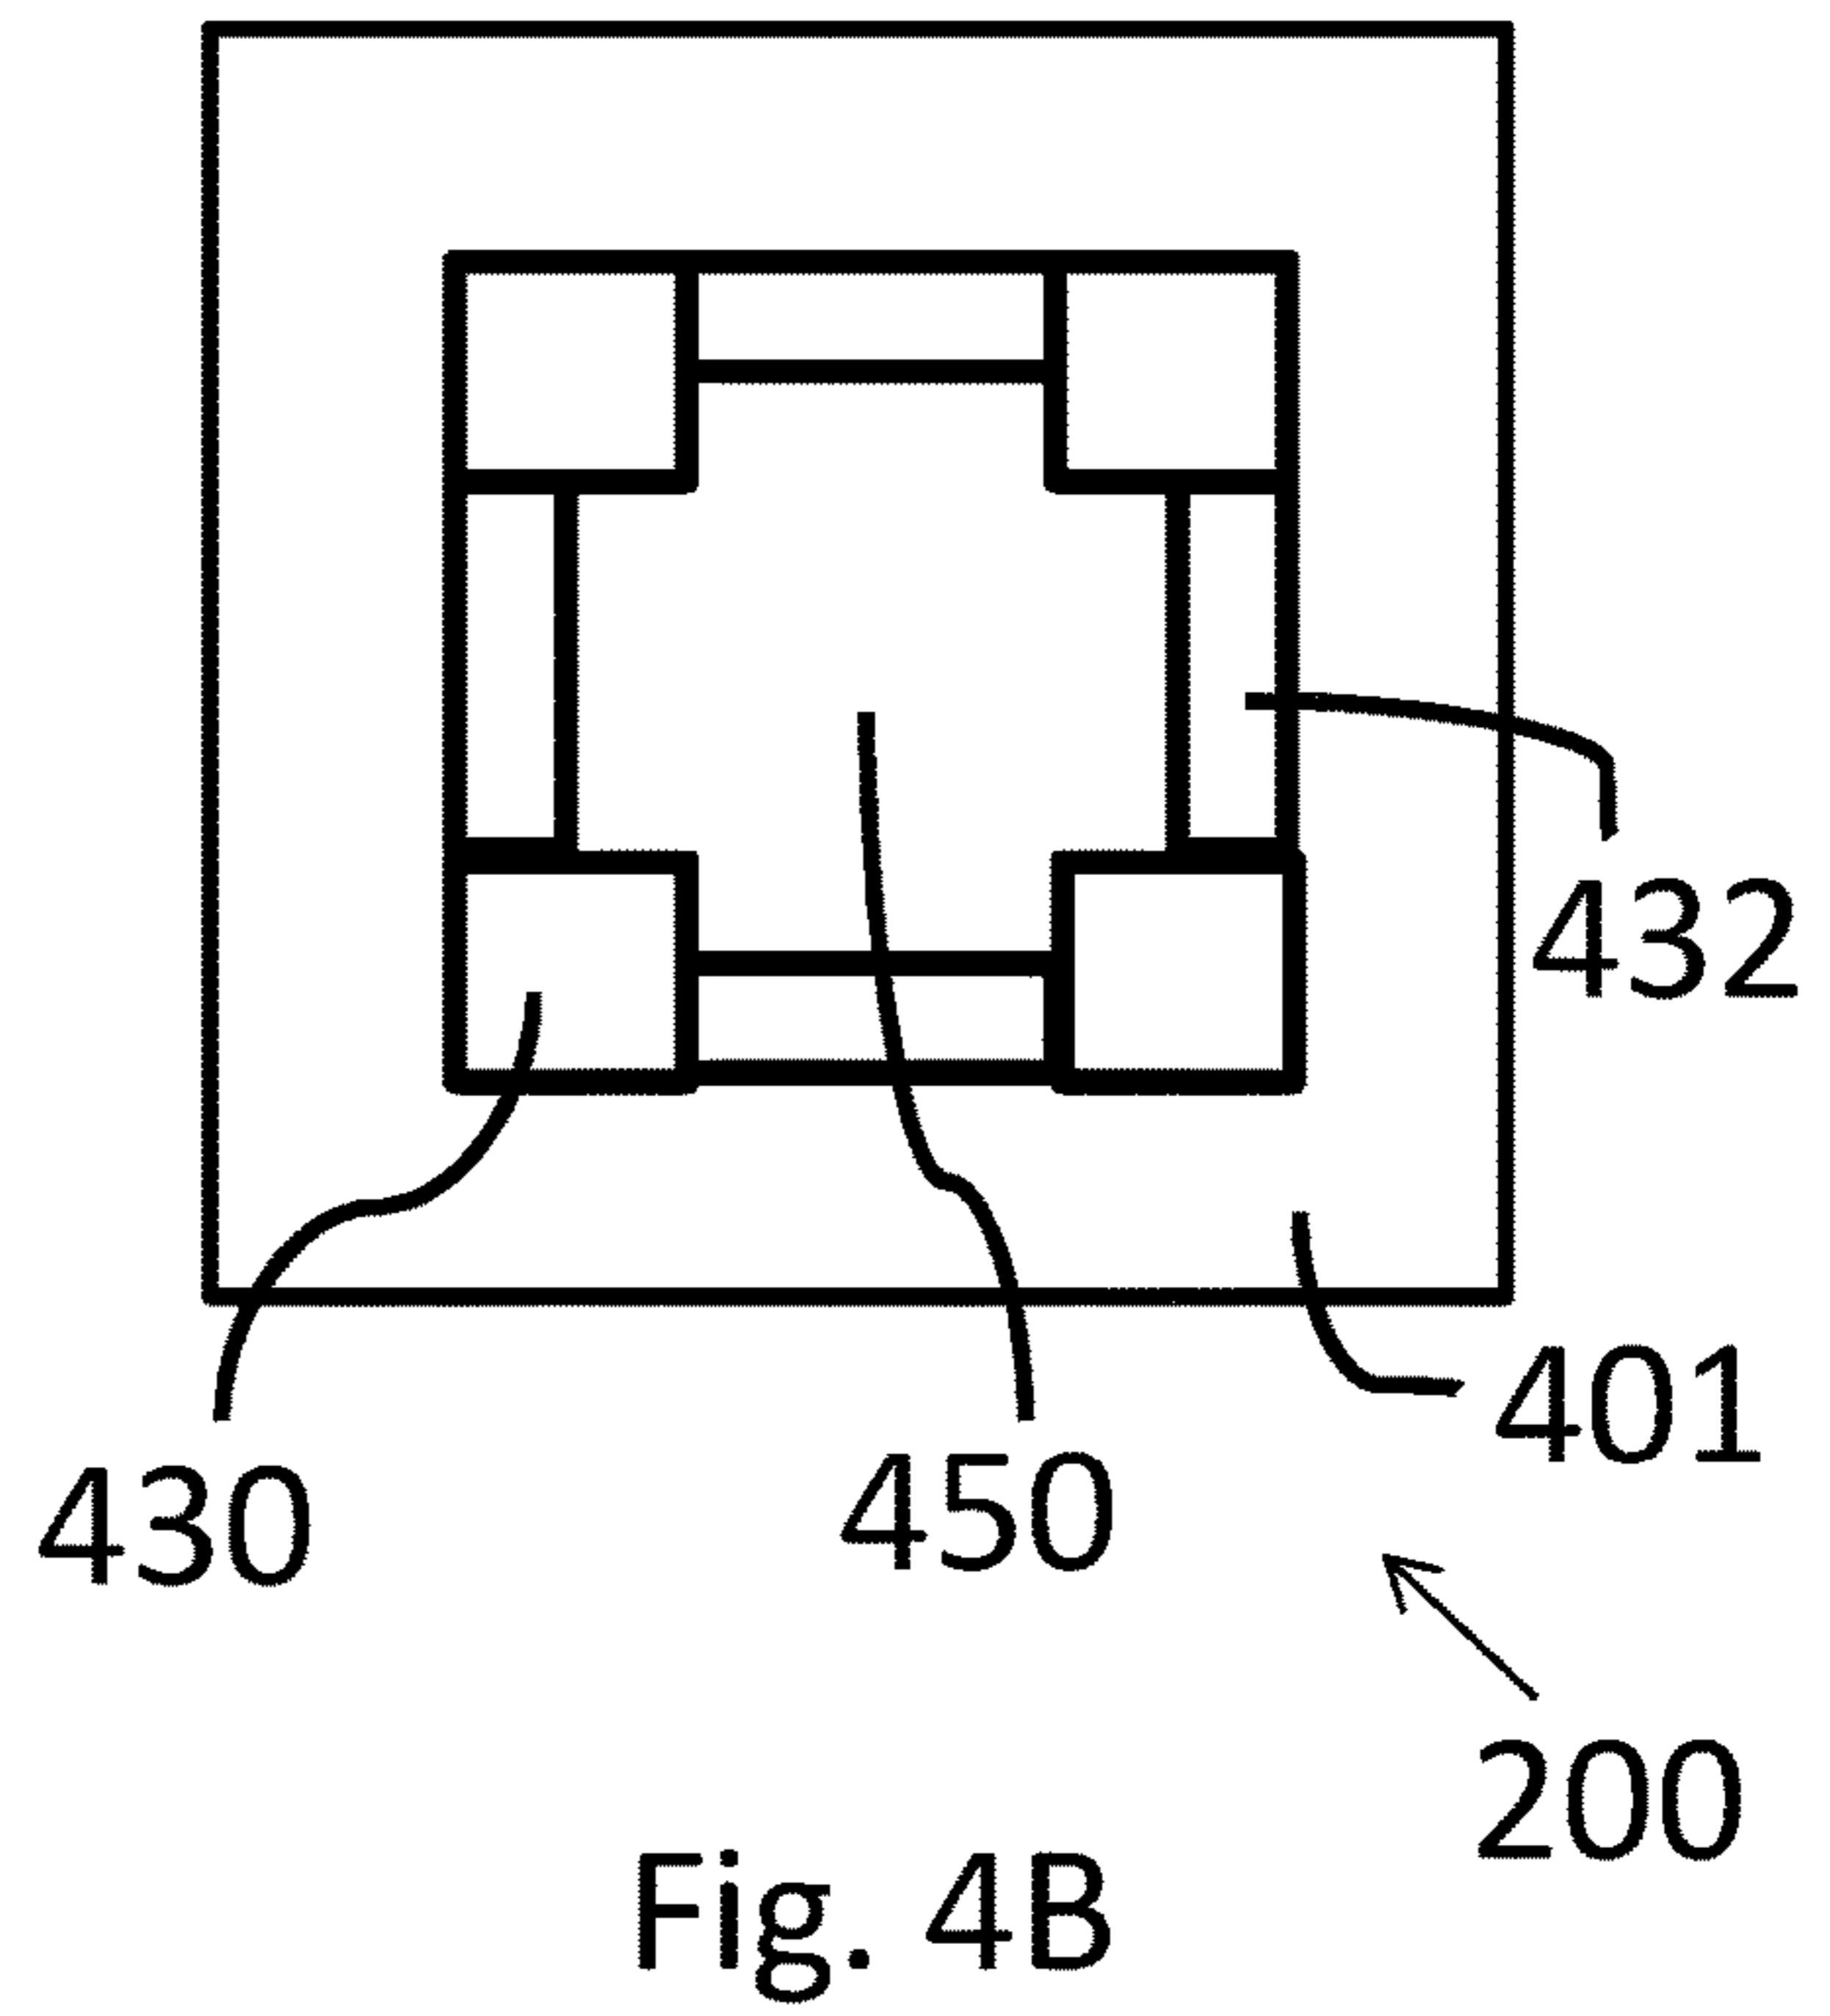
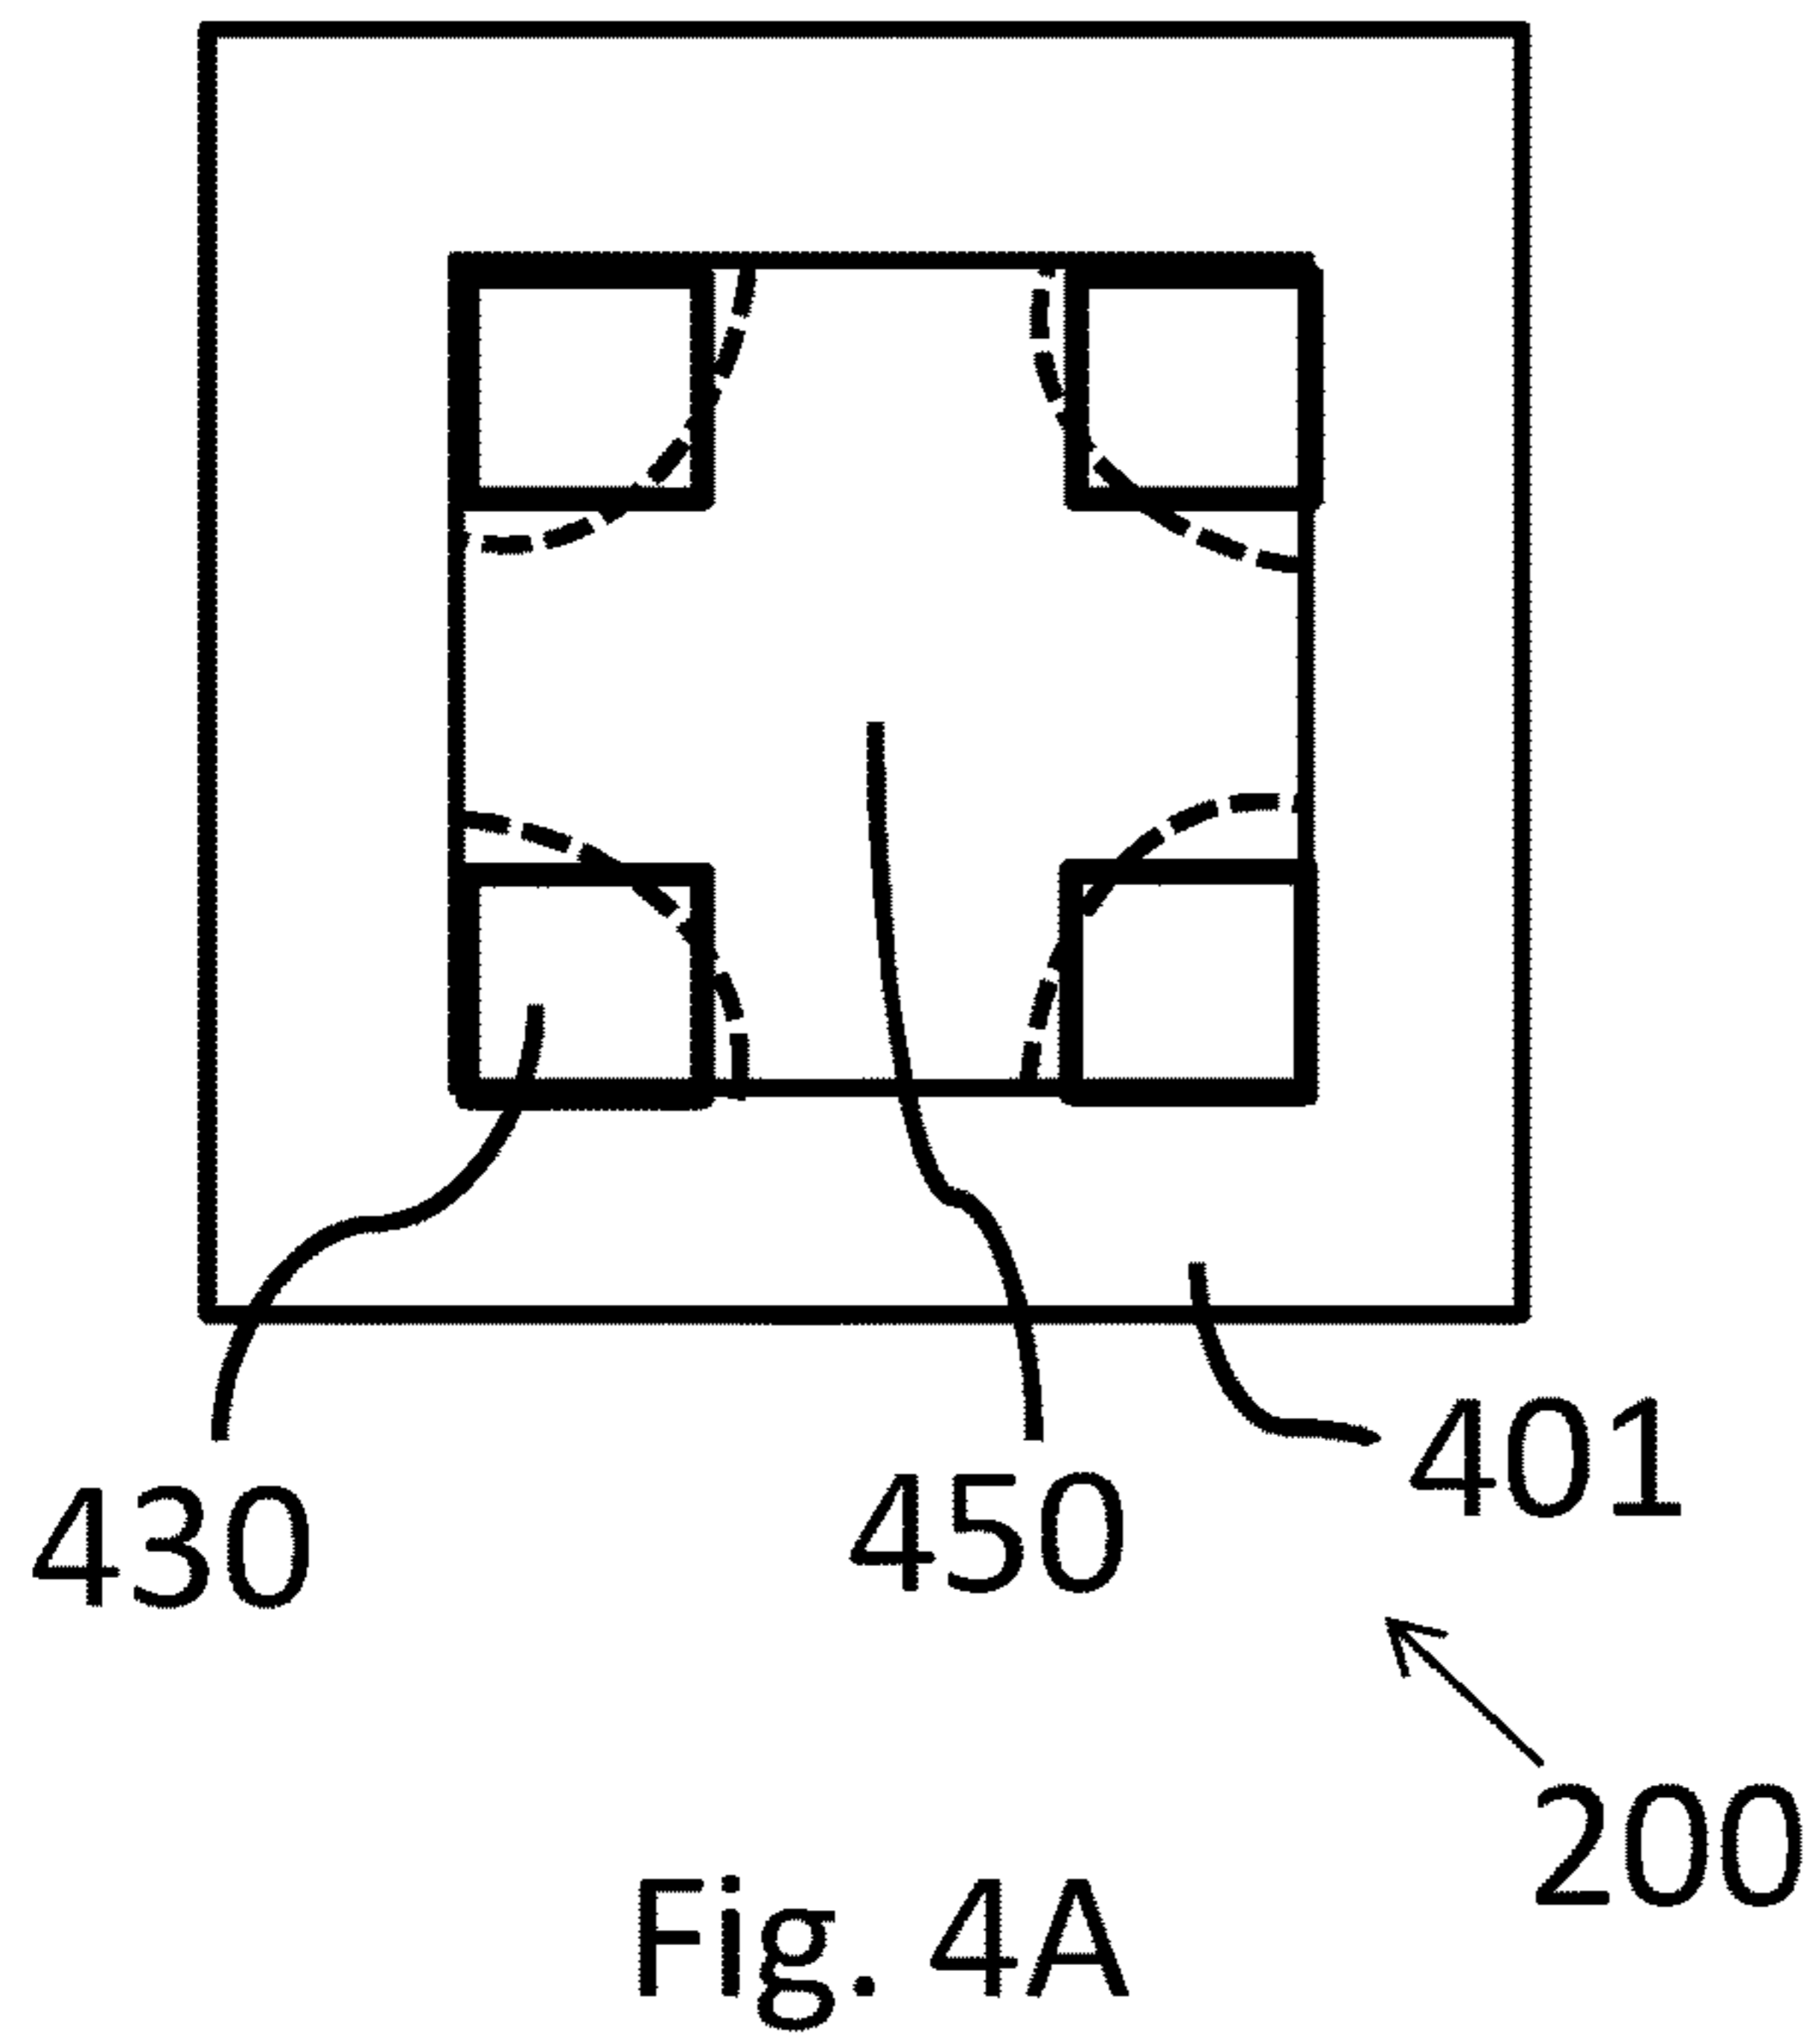


Fig. 3



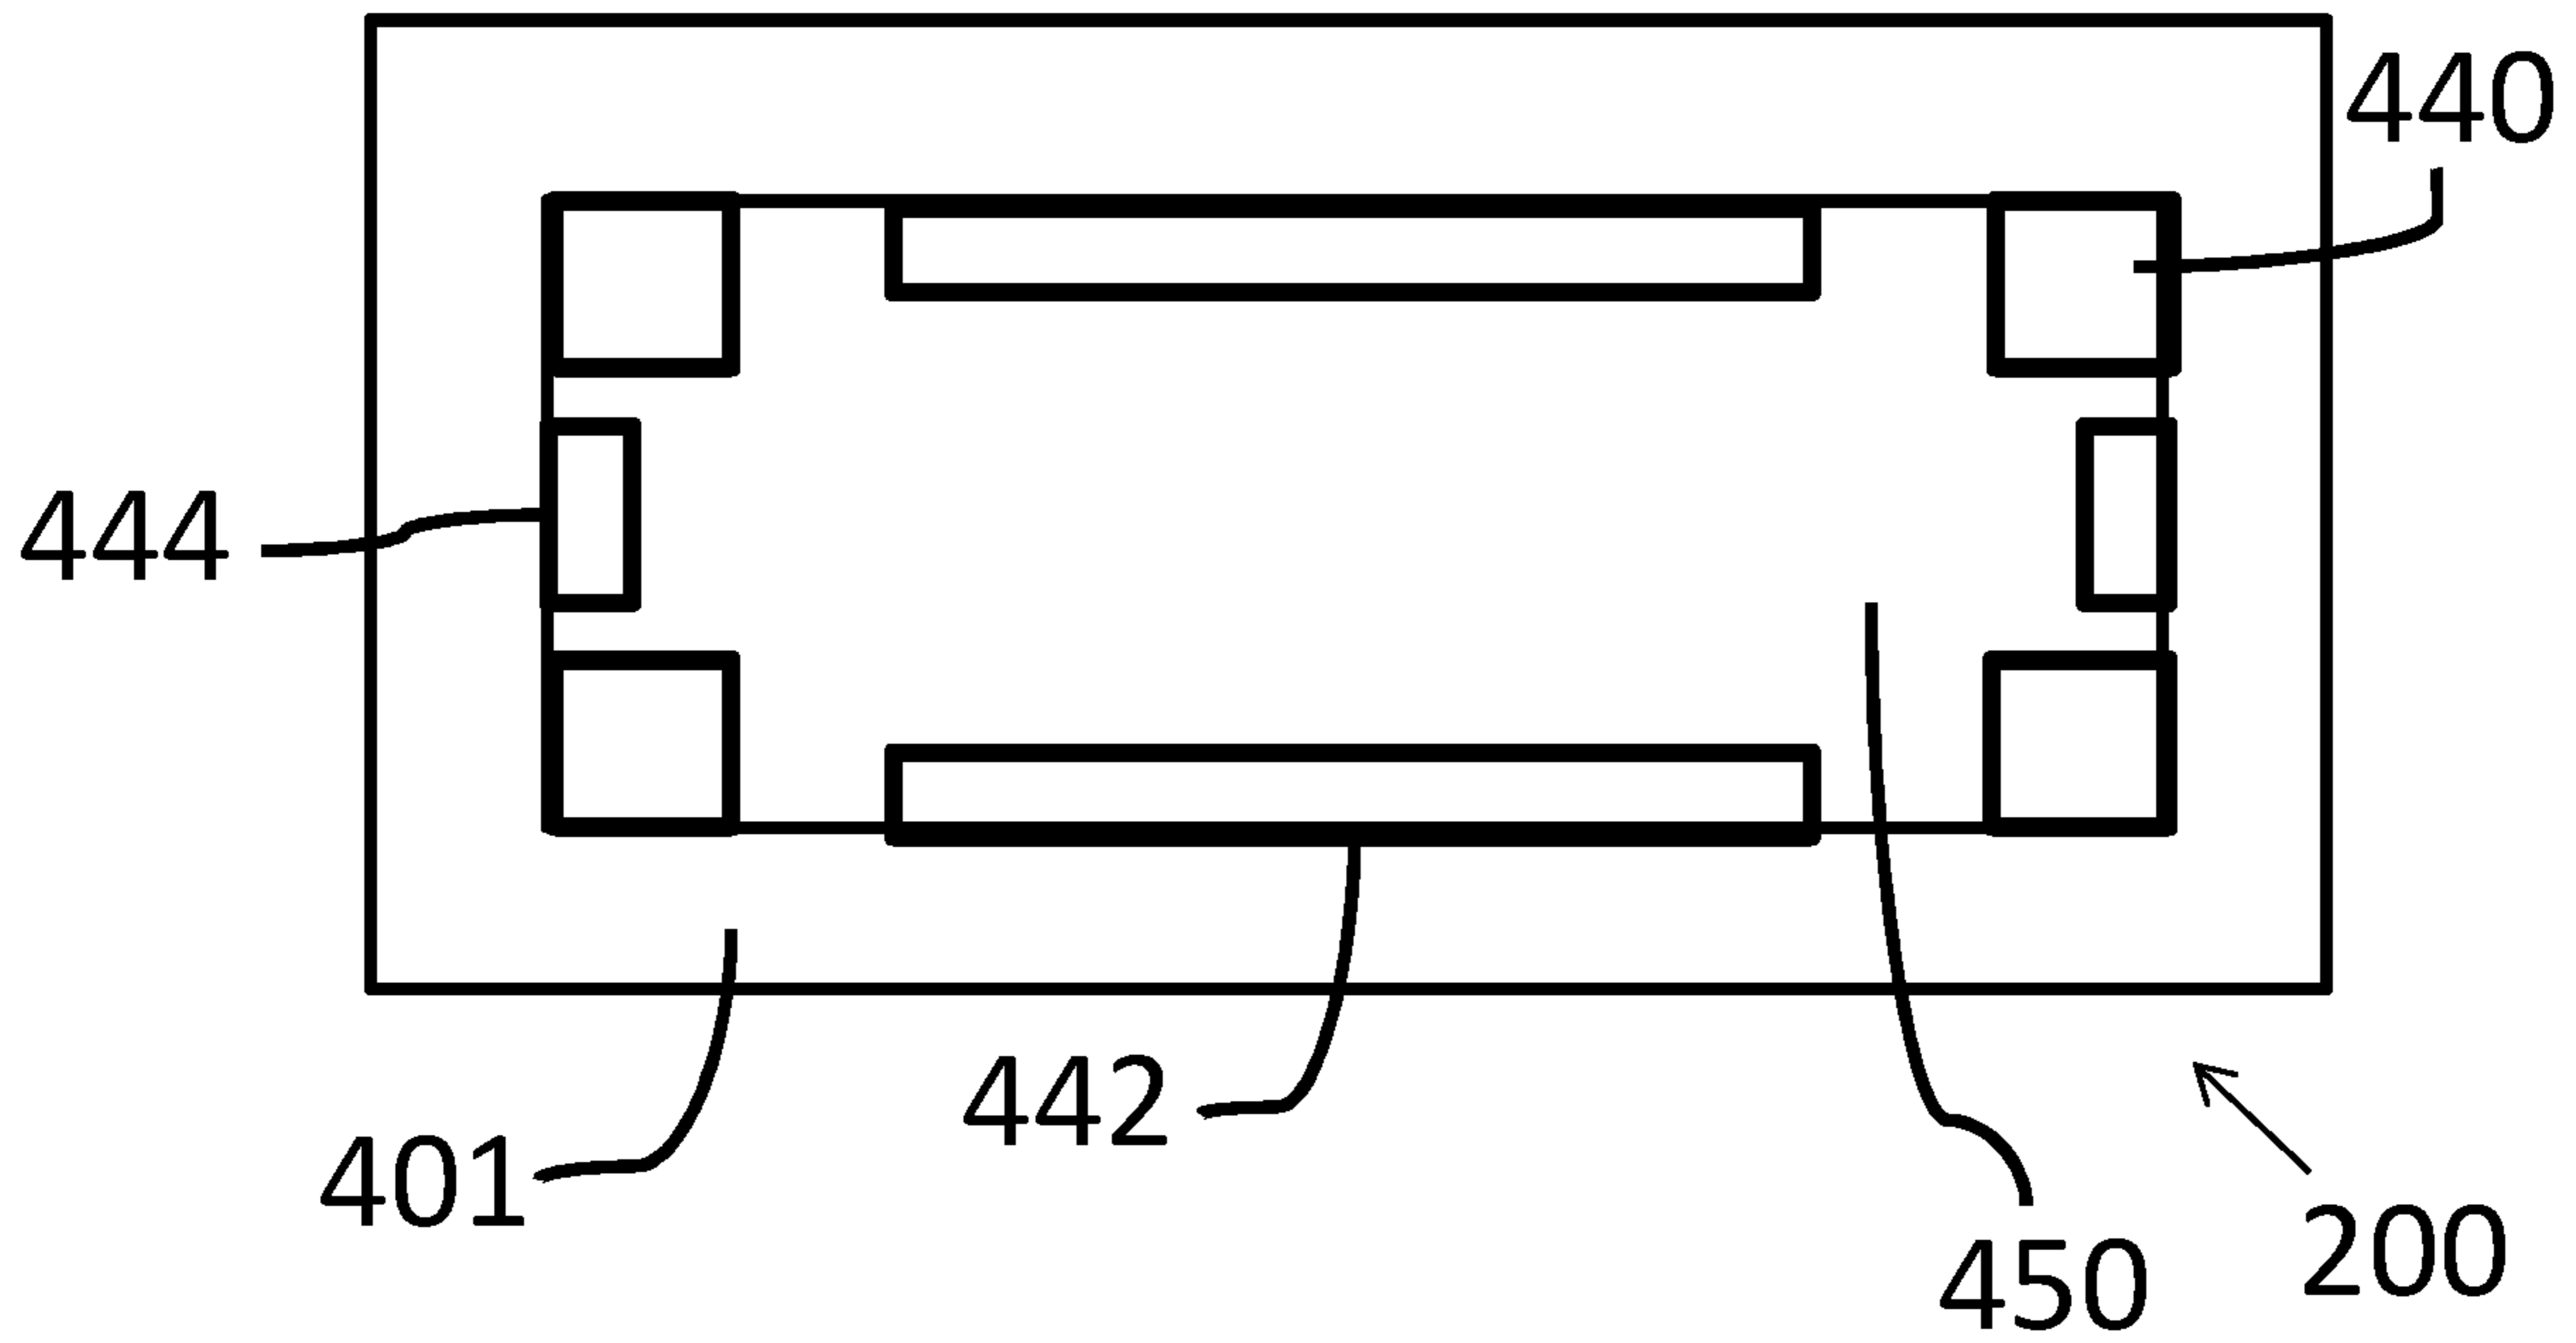


Fig. 4D

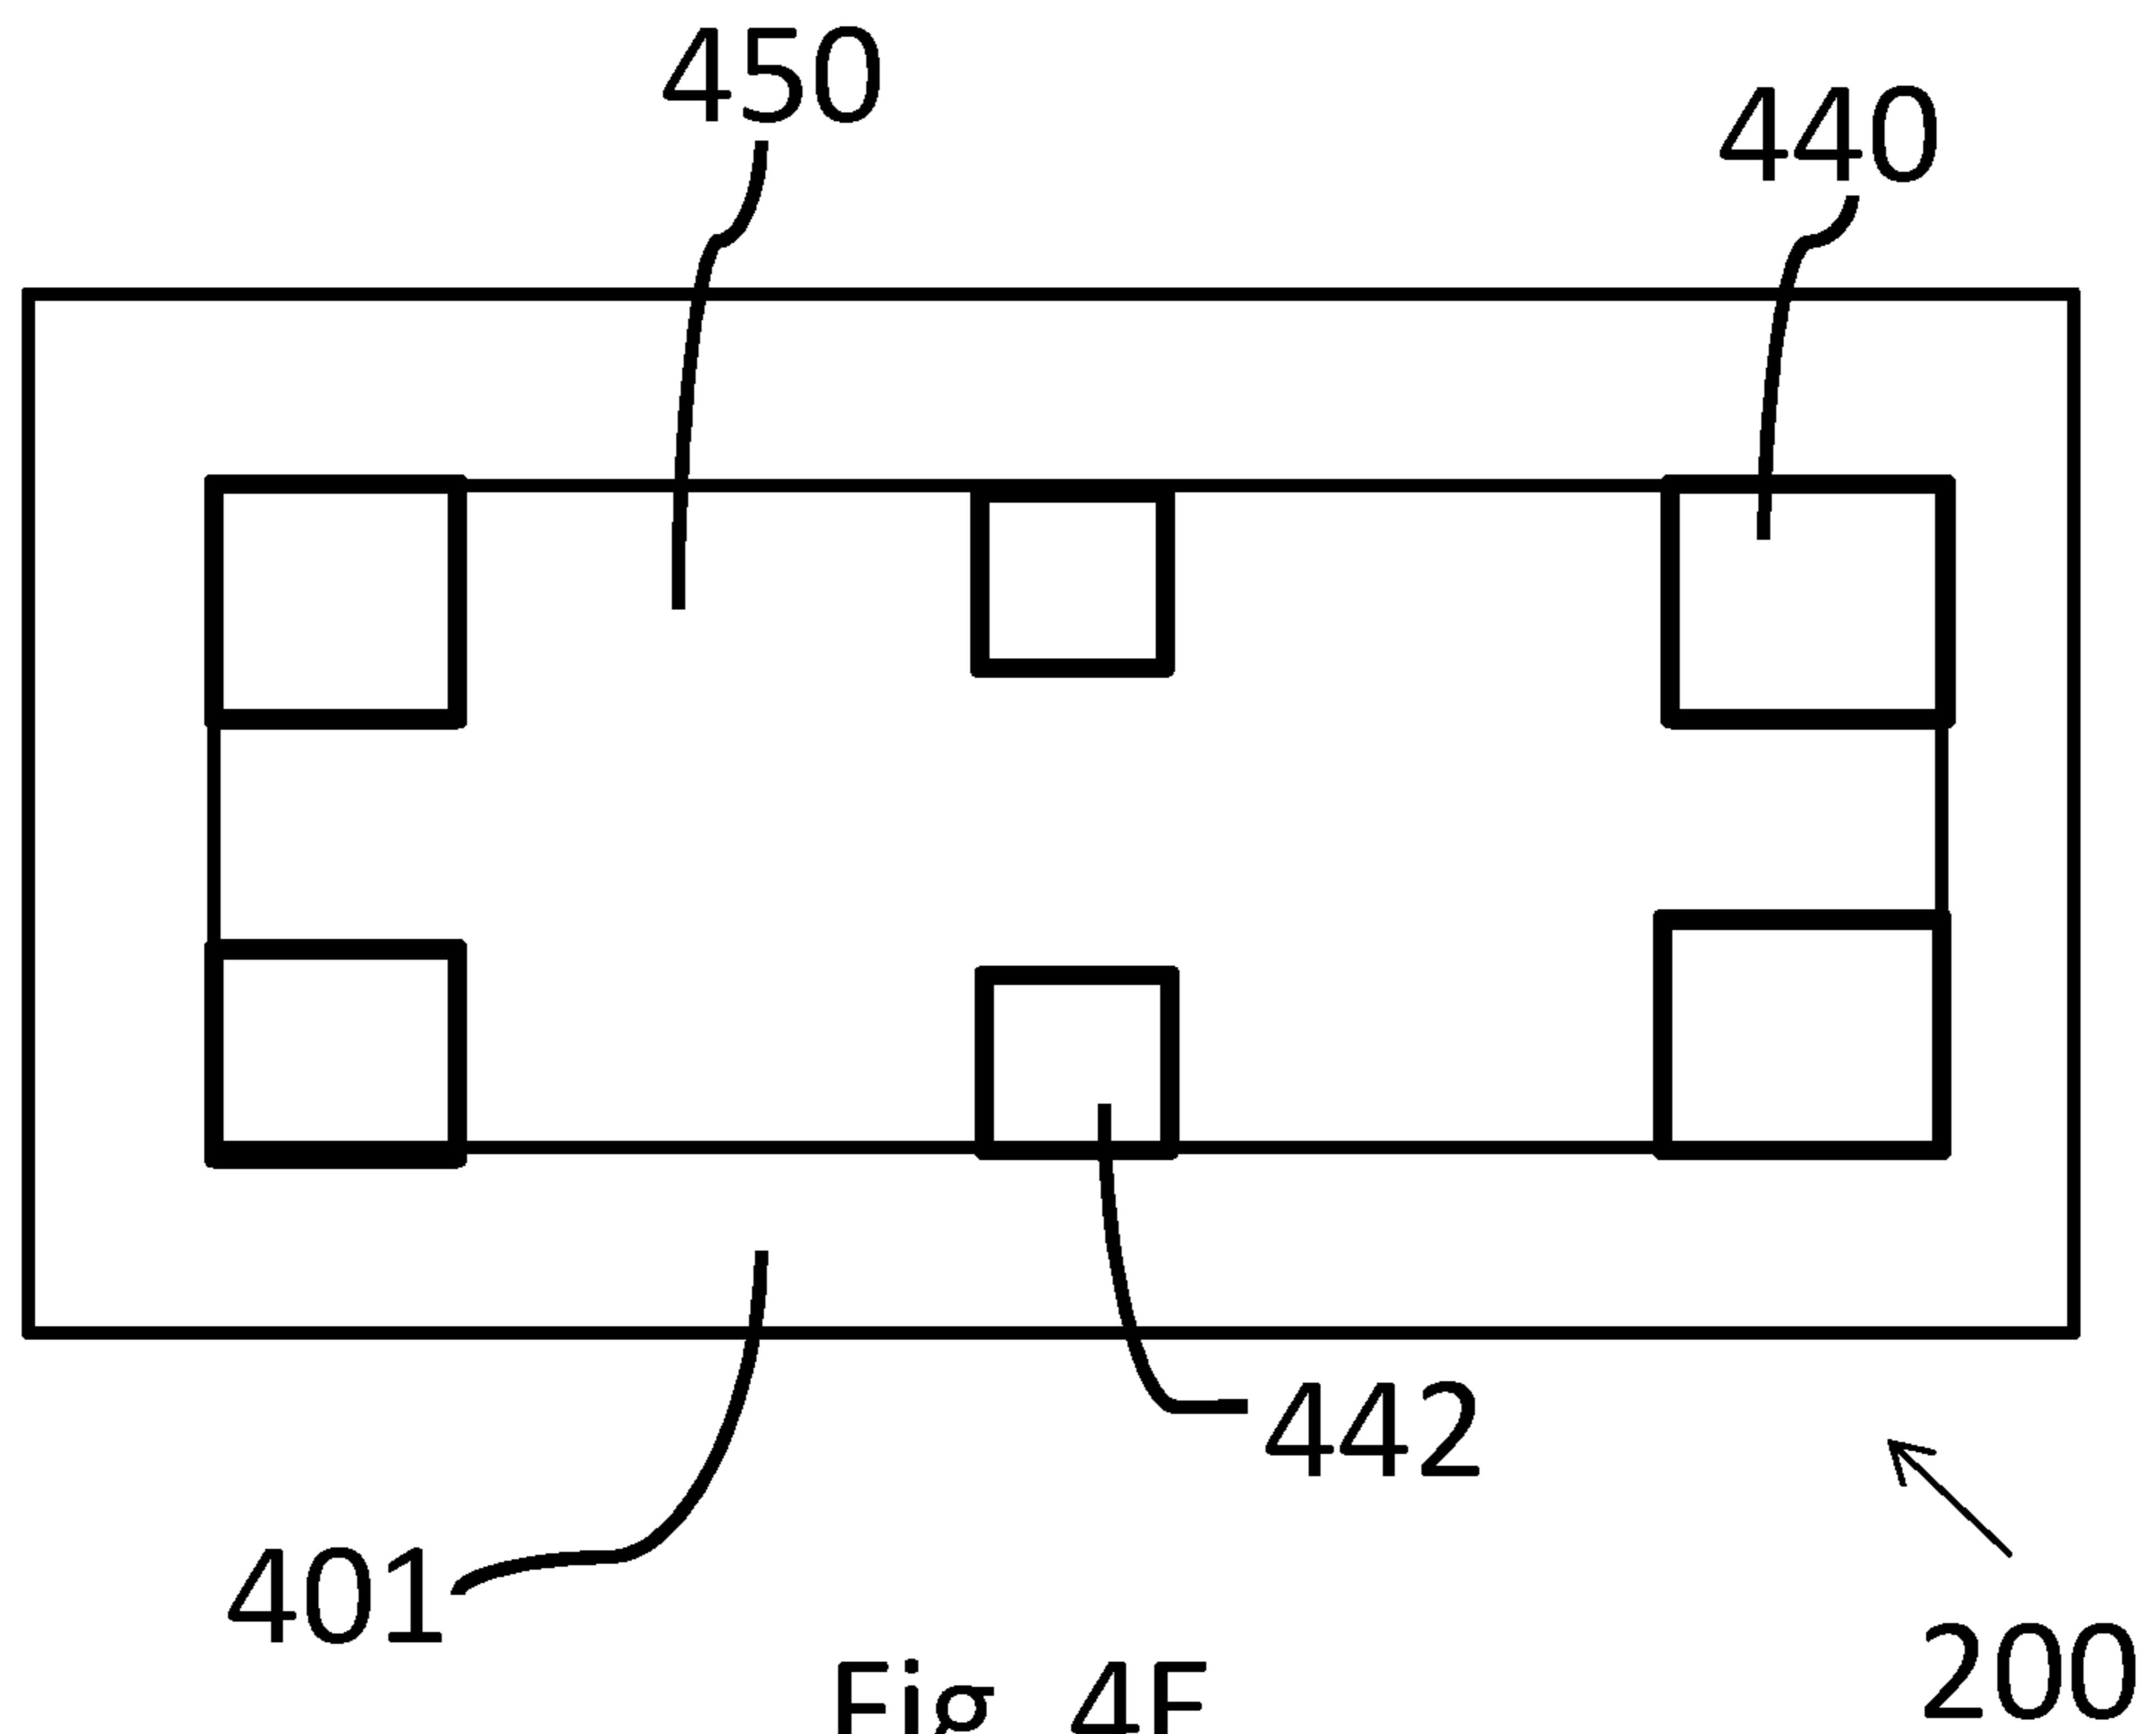
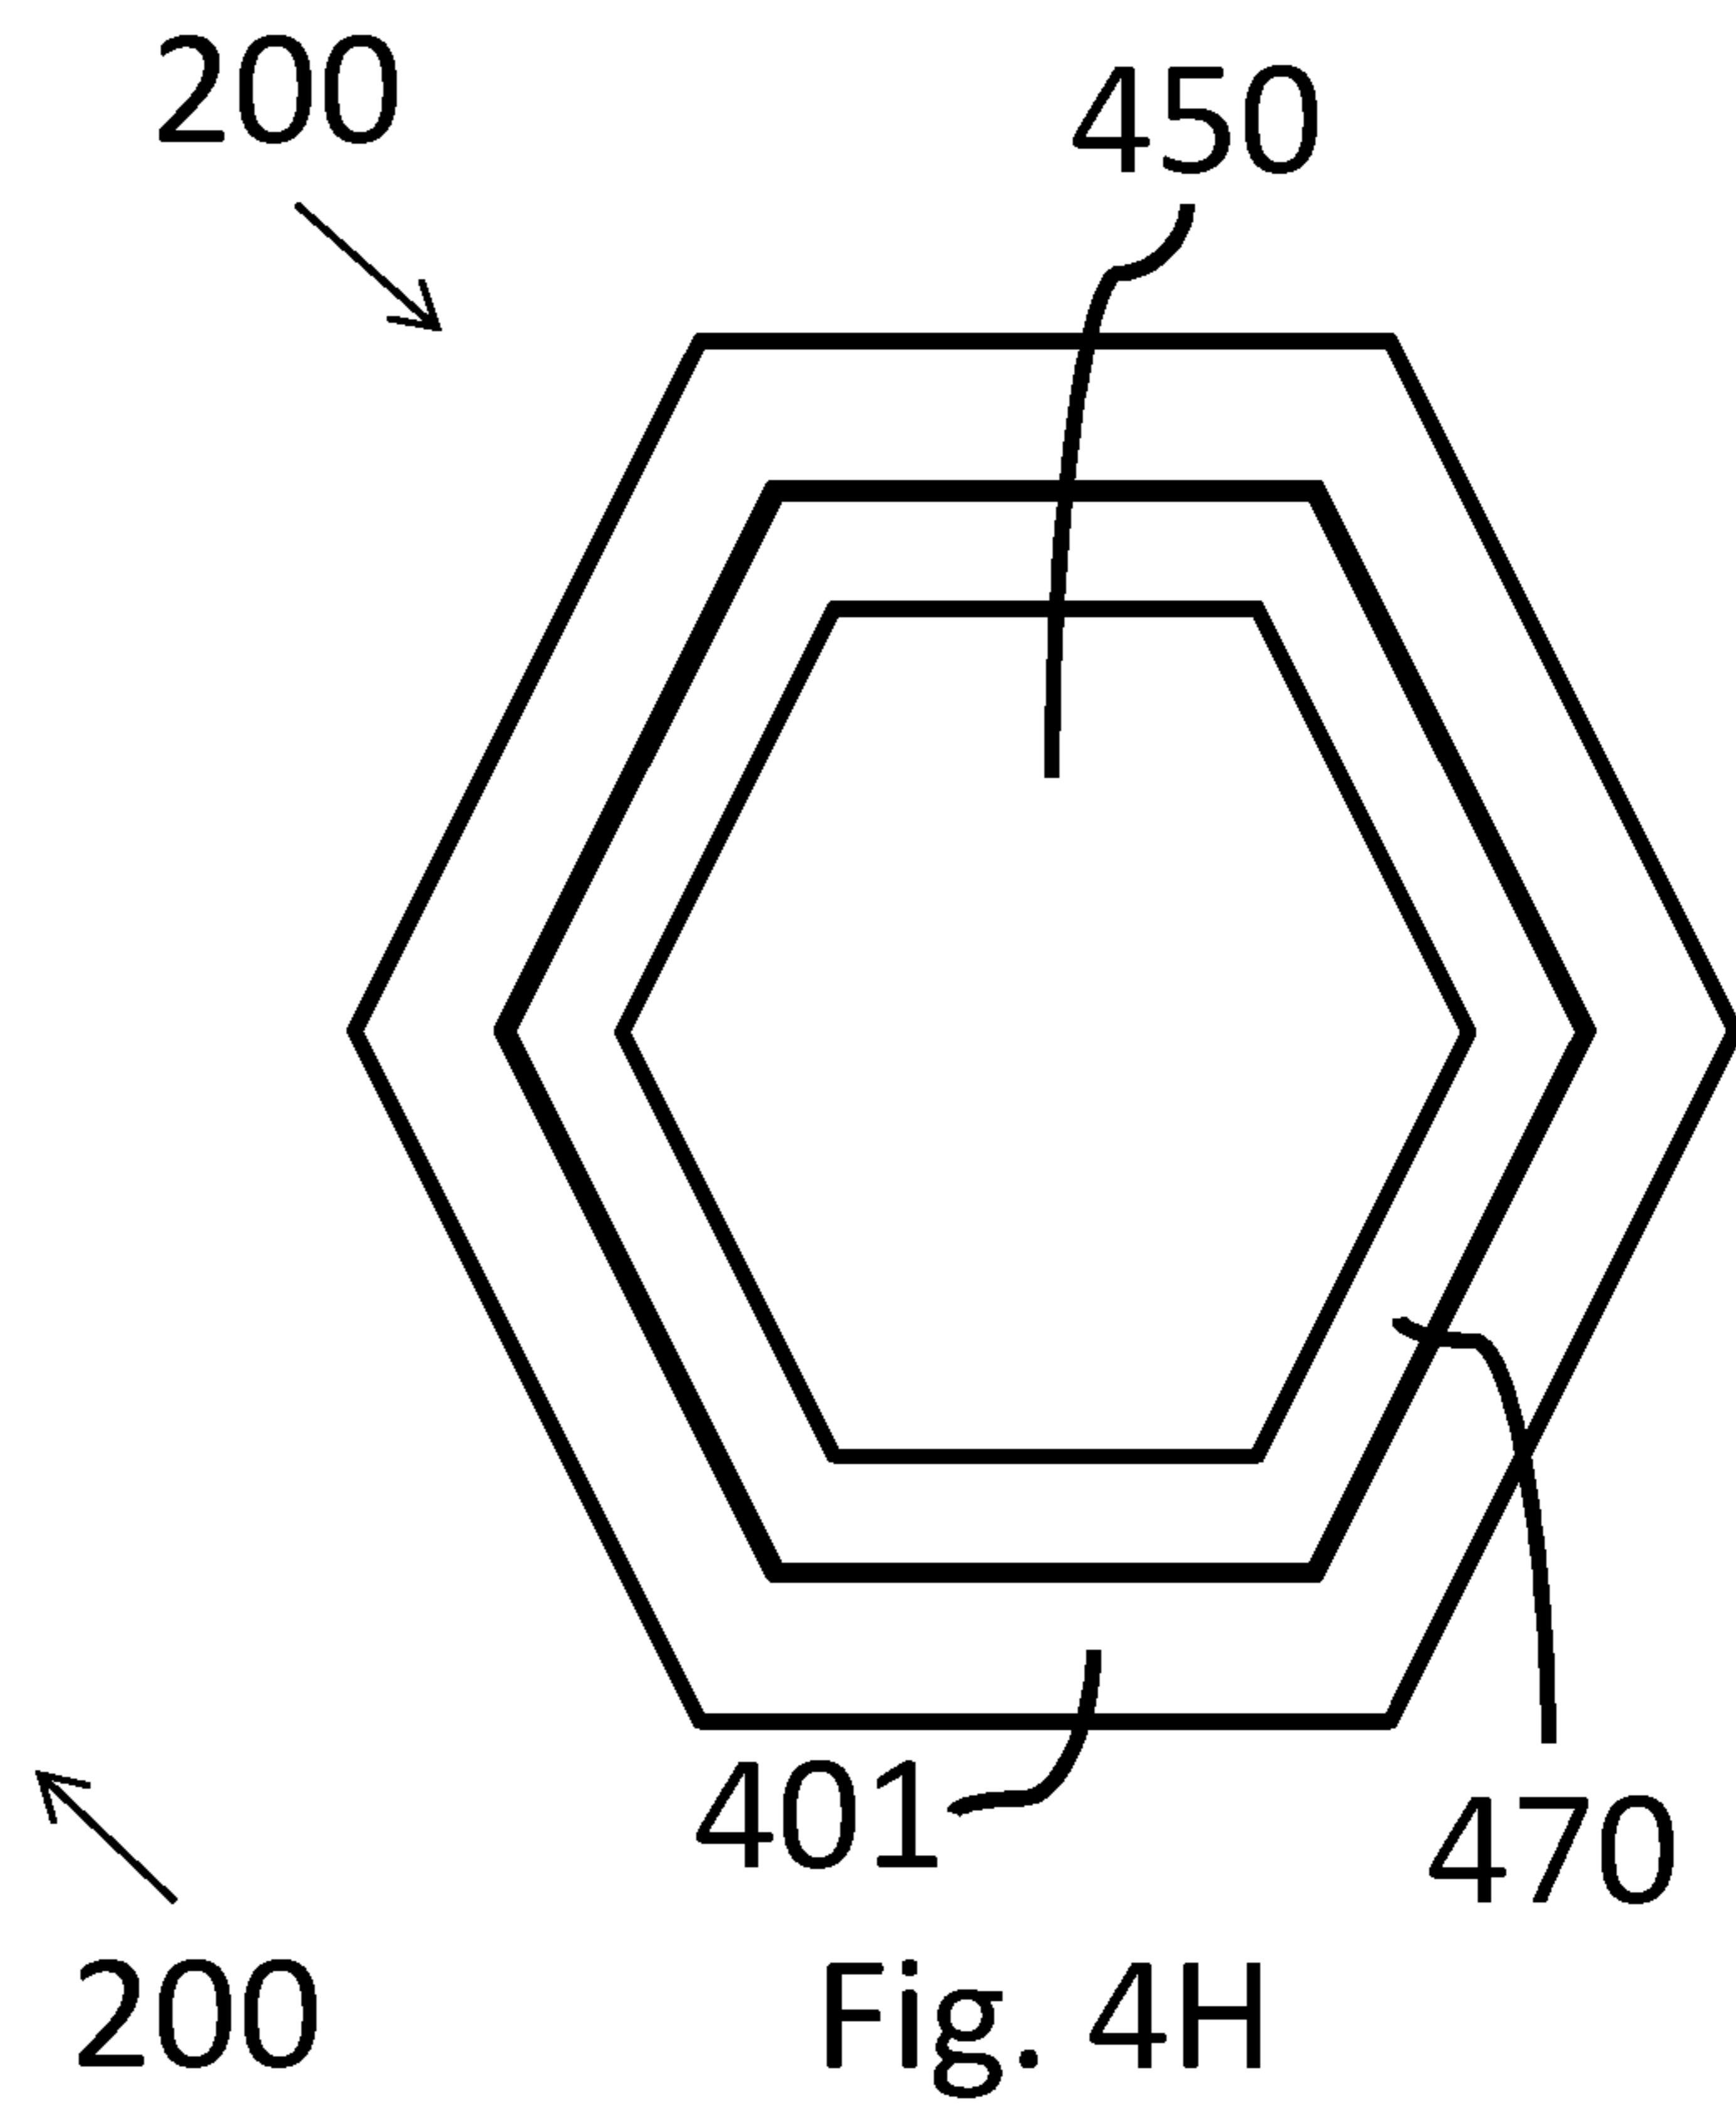
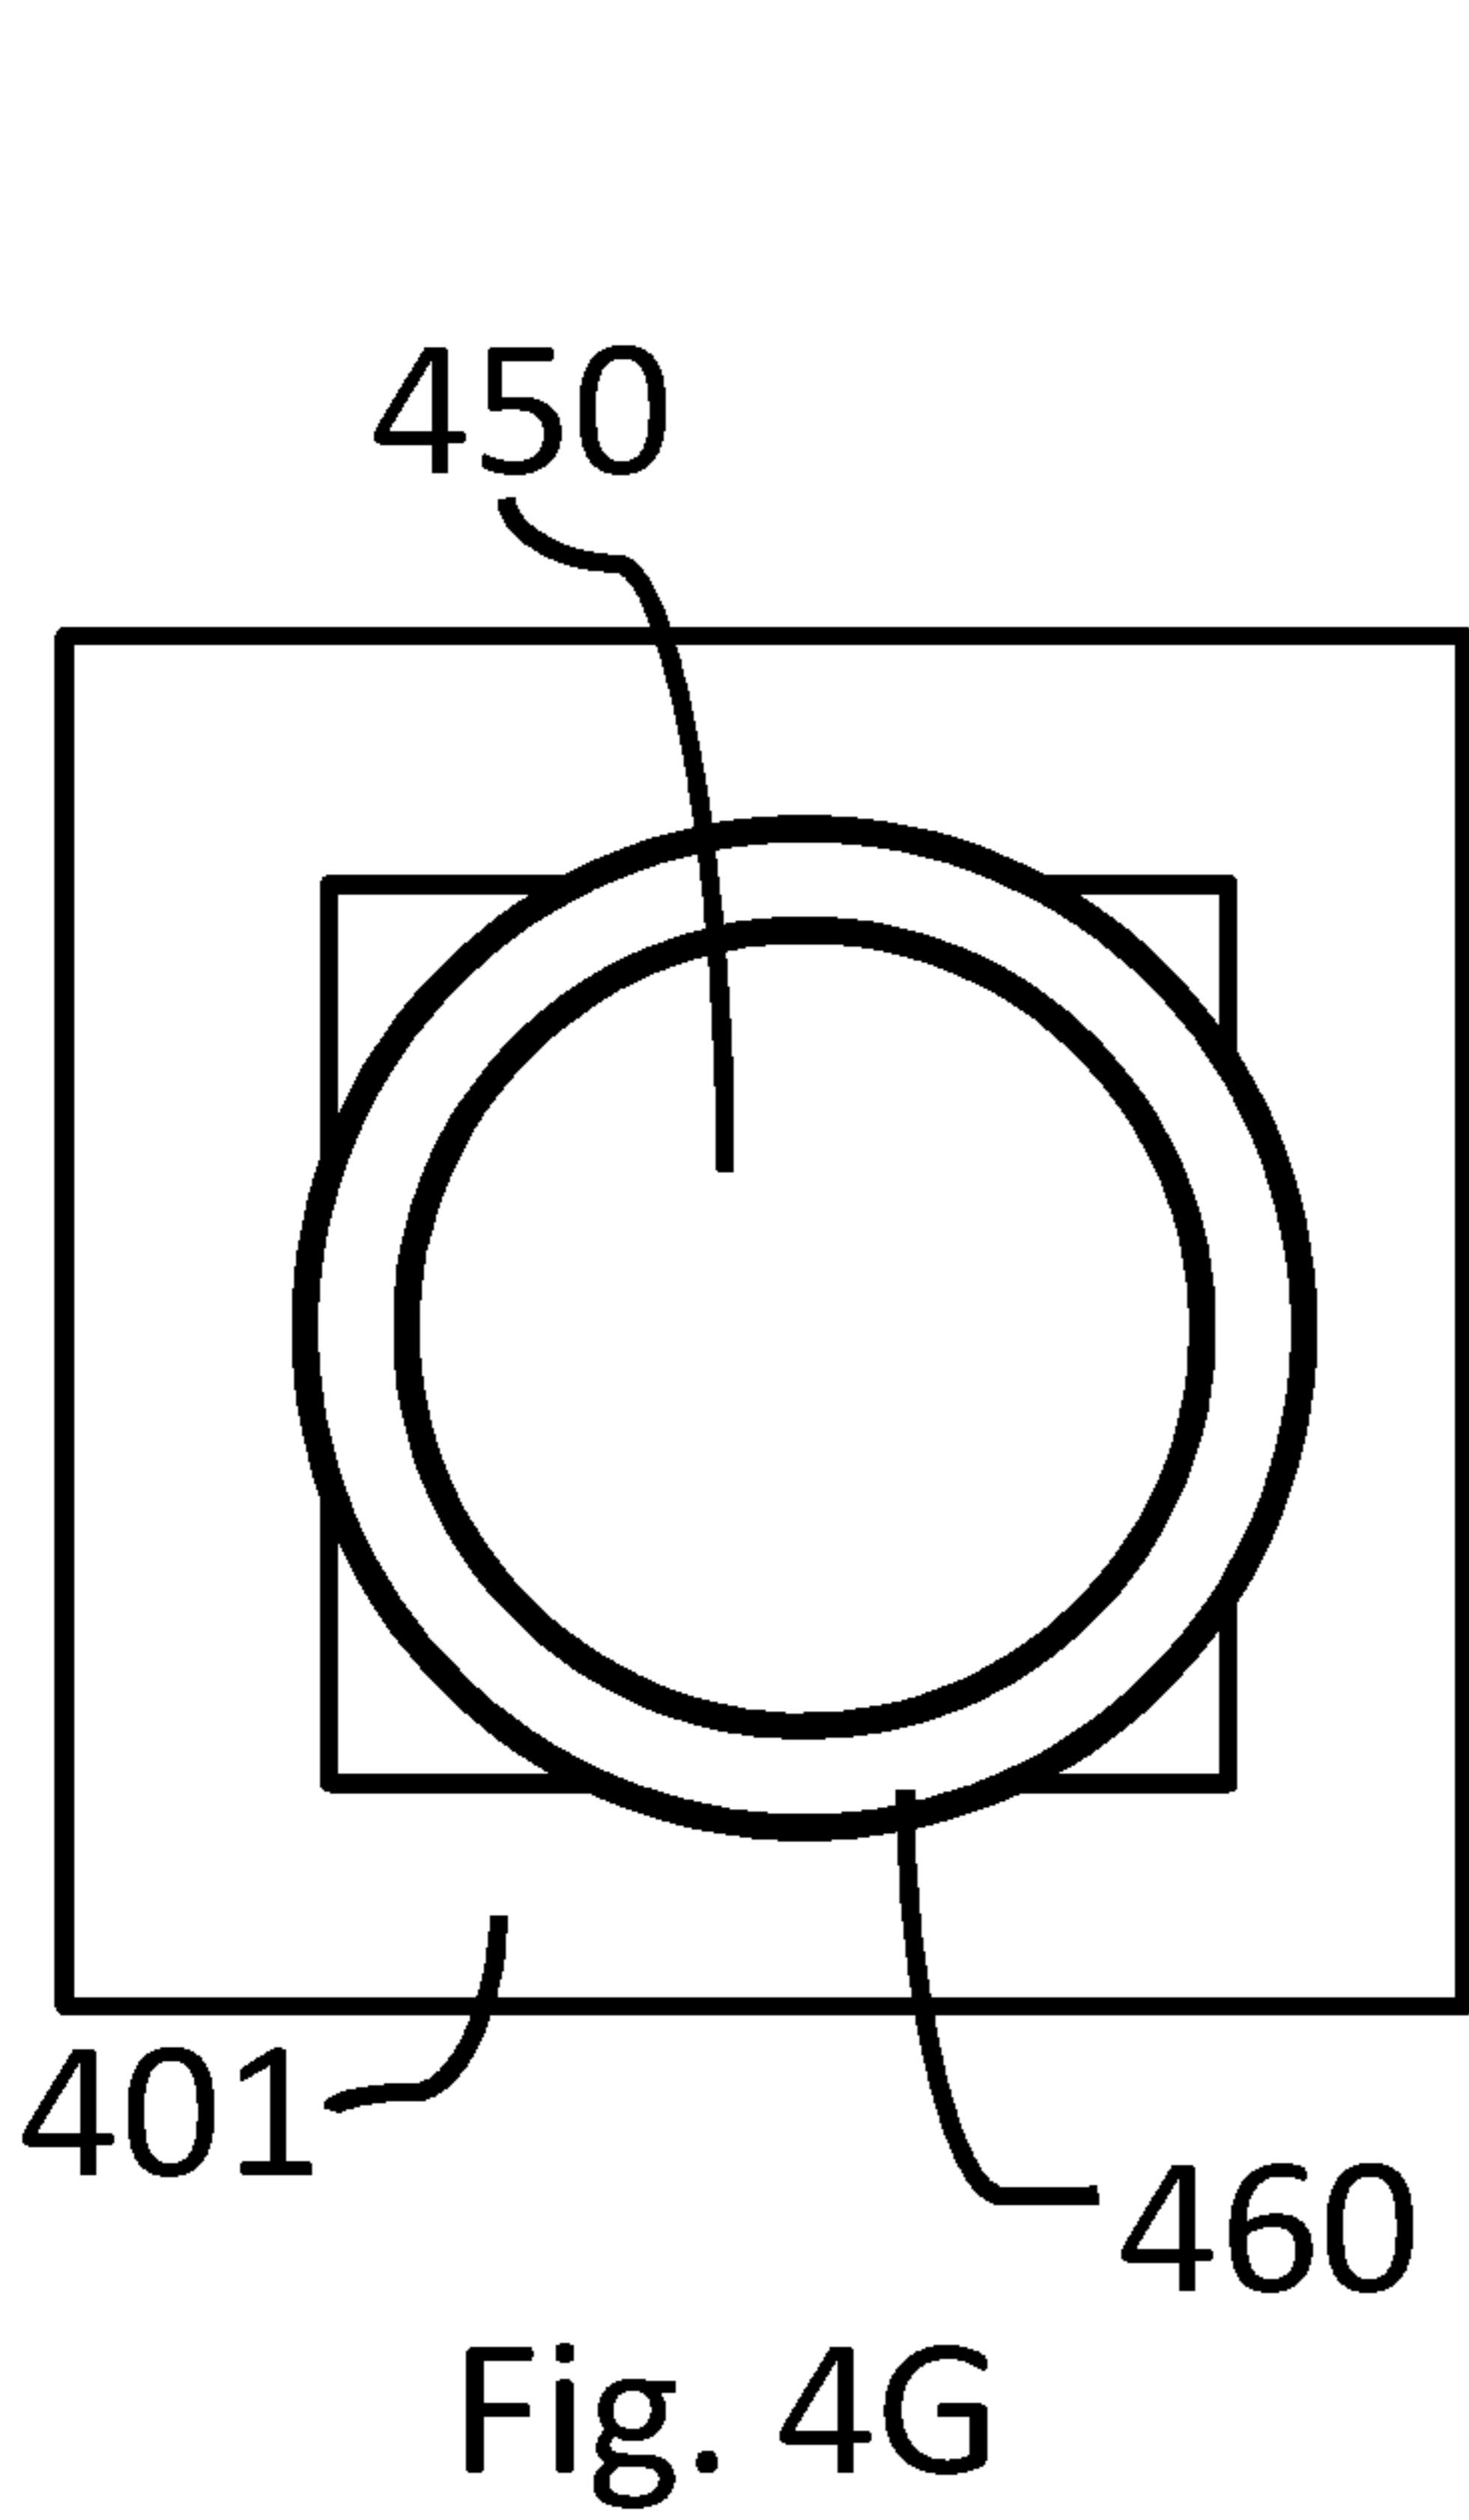
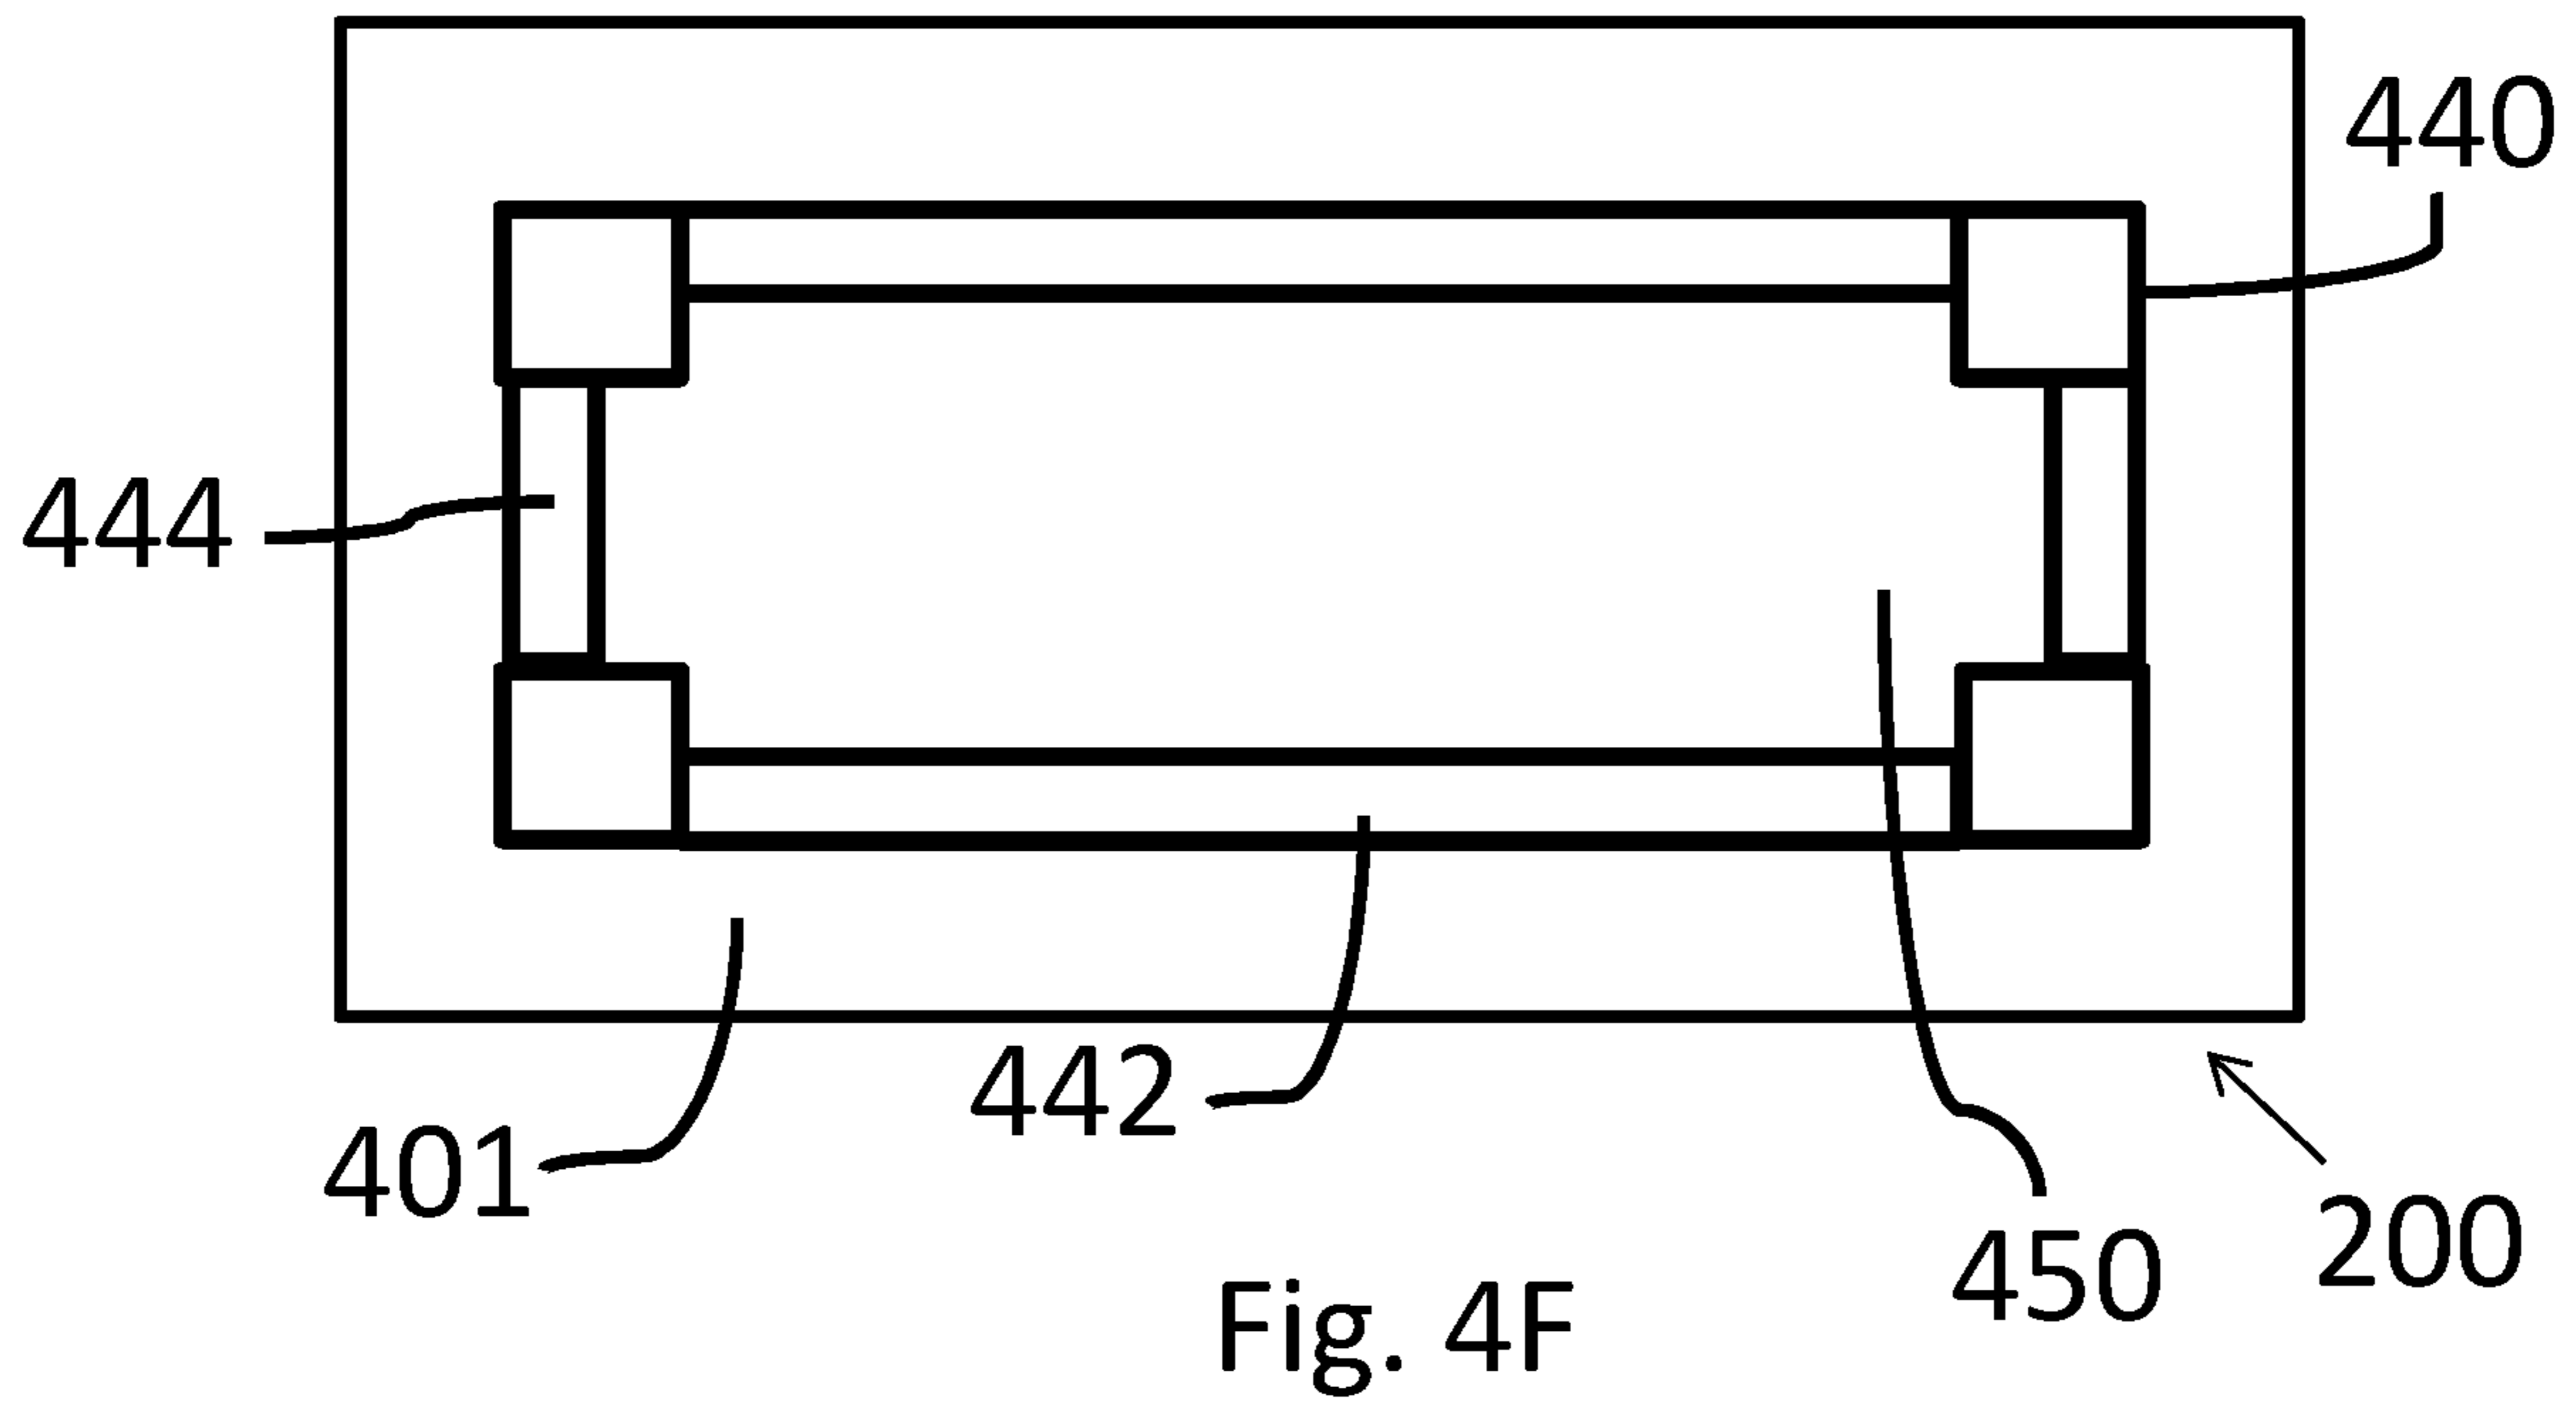


Fig. 4E



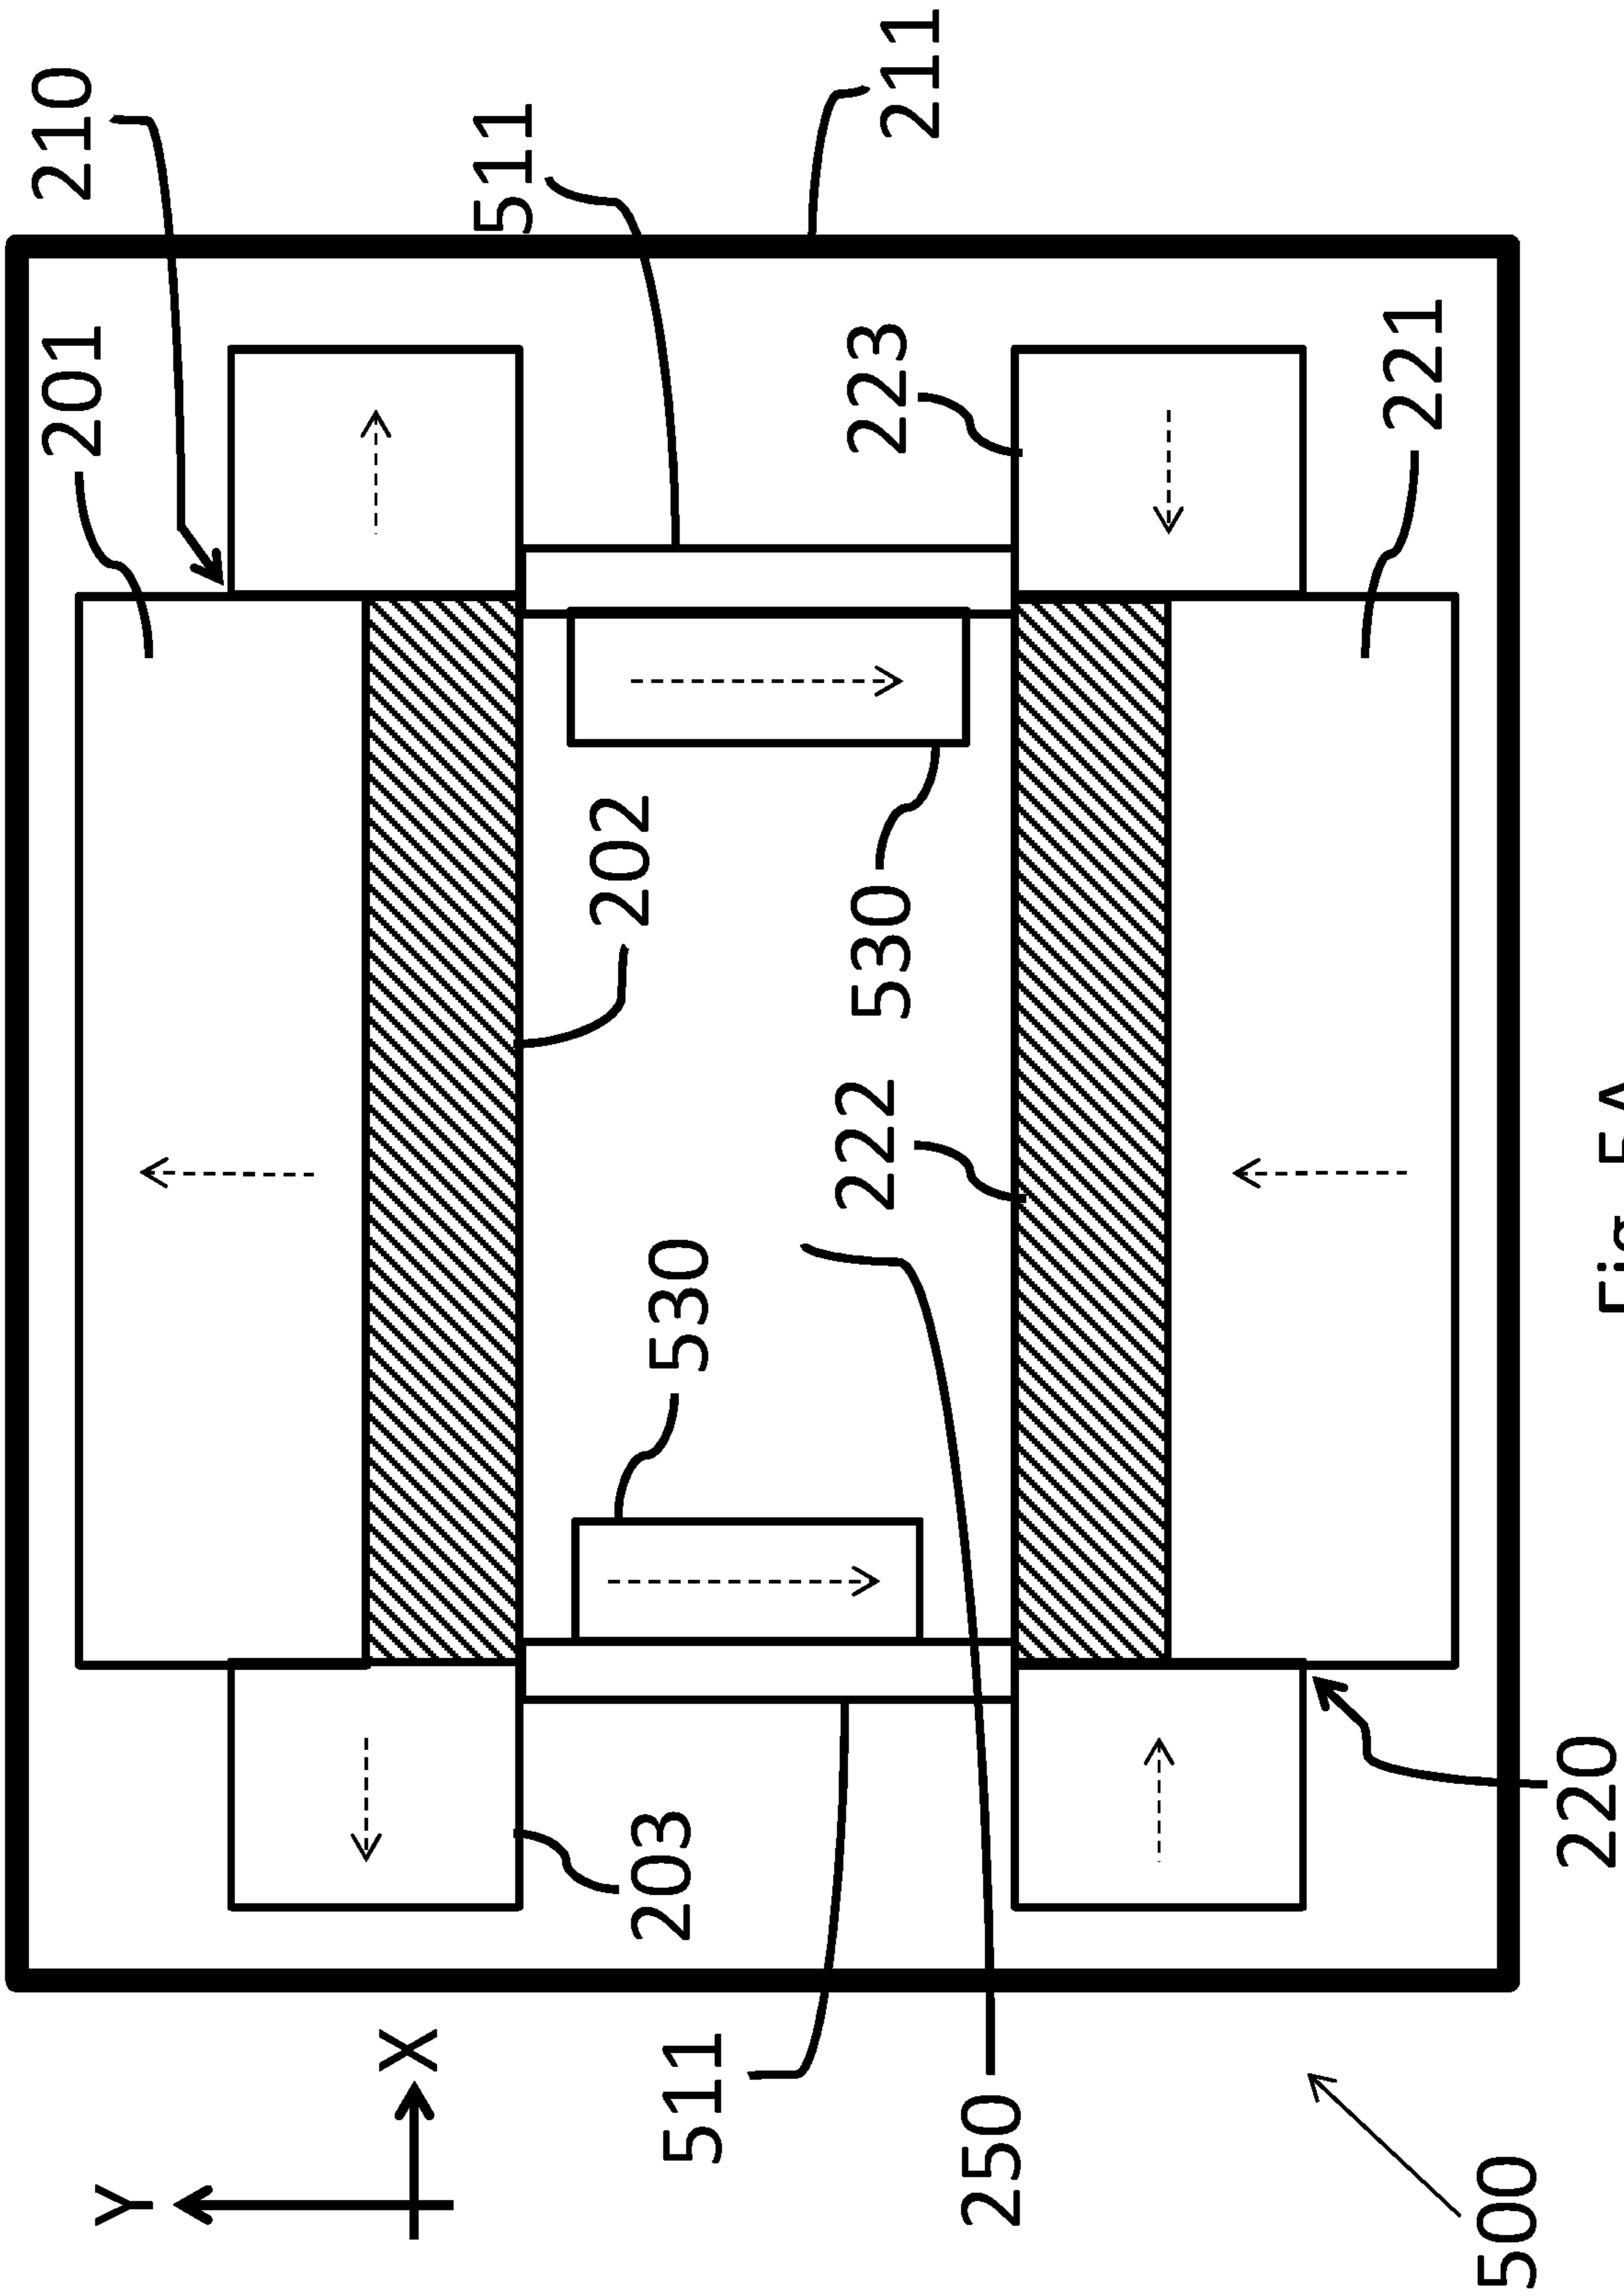


Fig. 5A

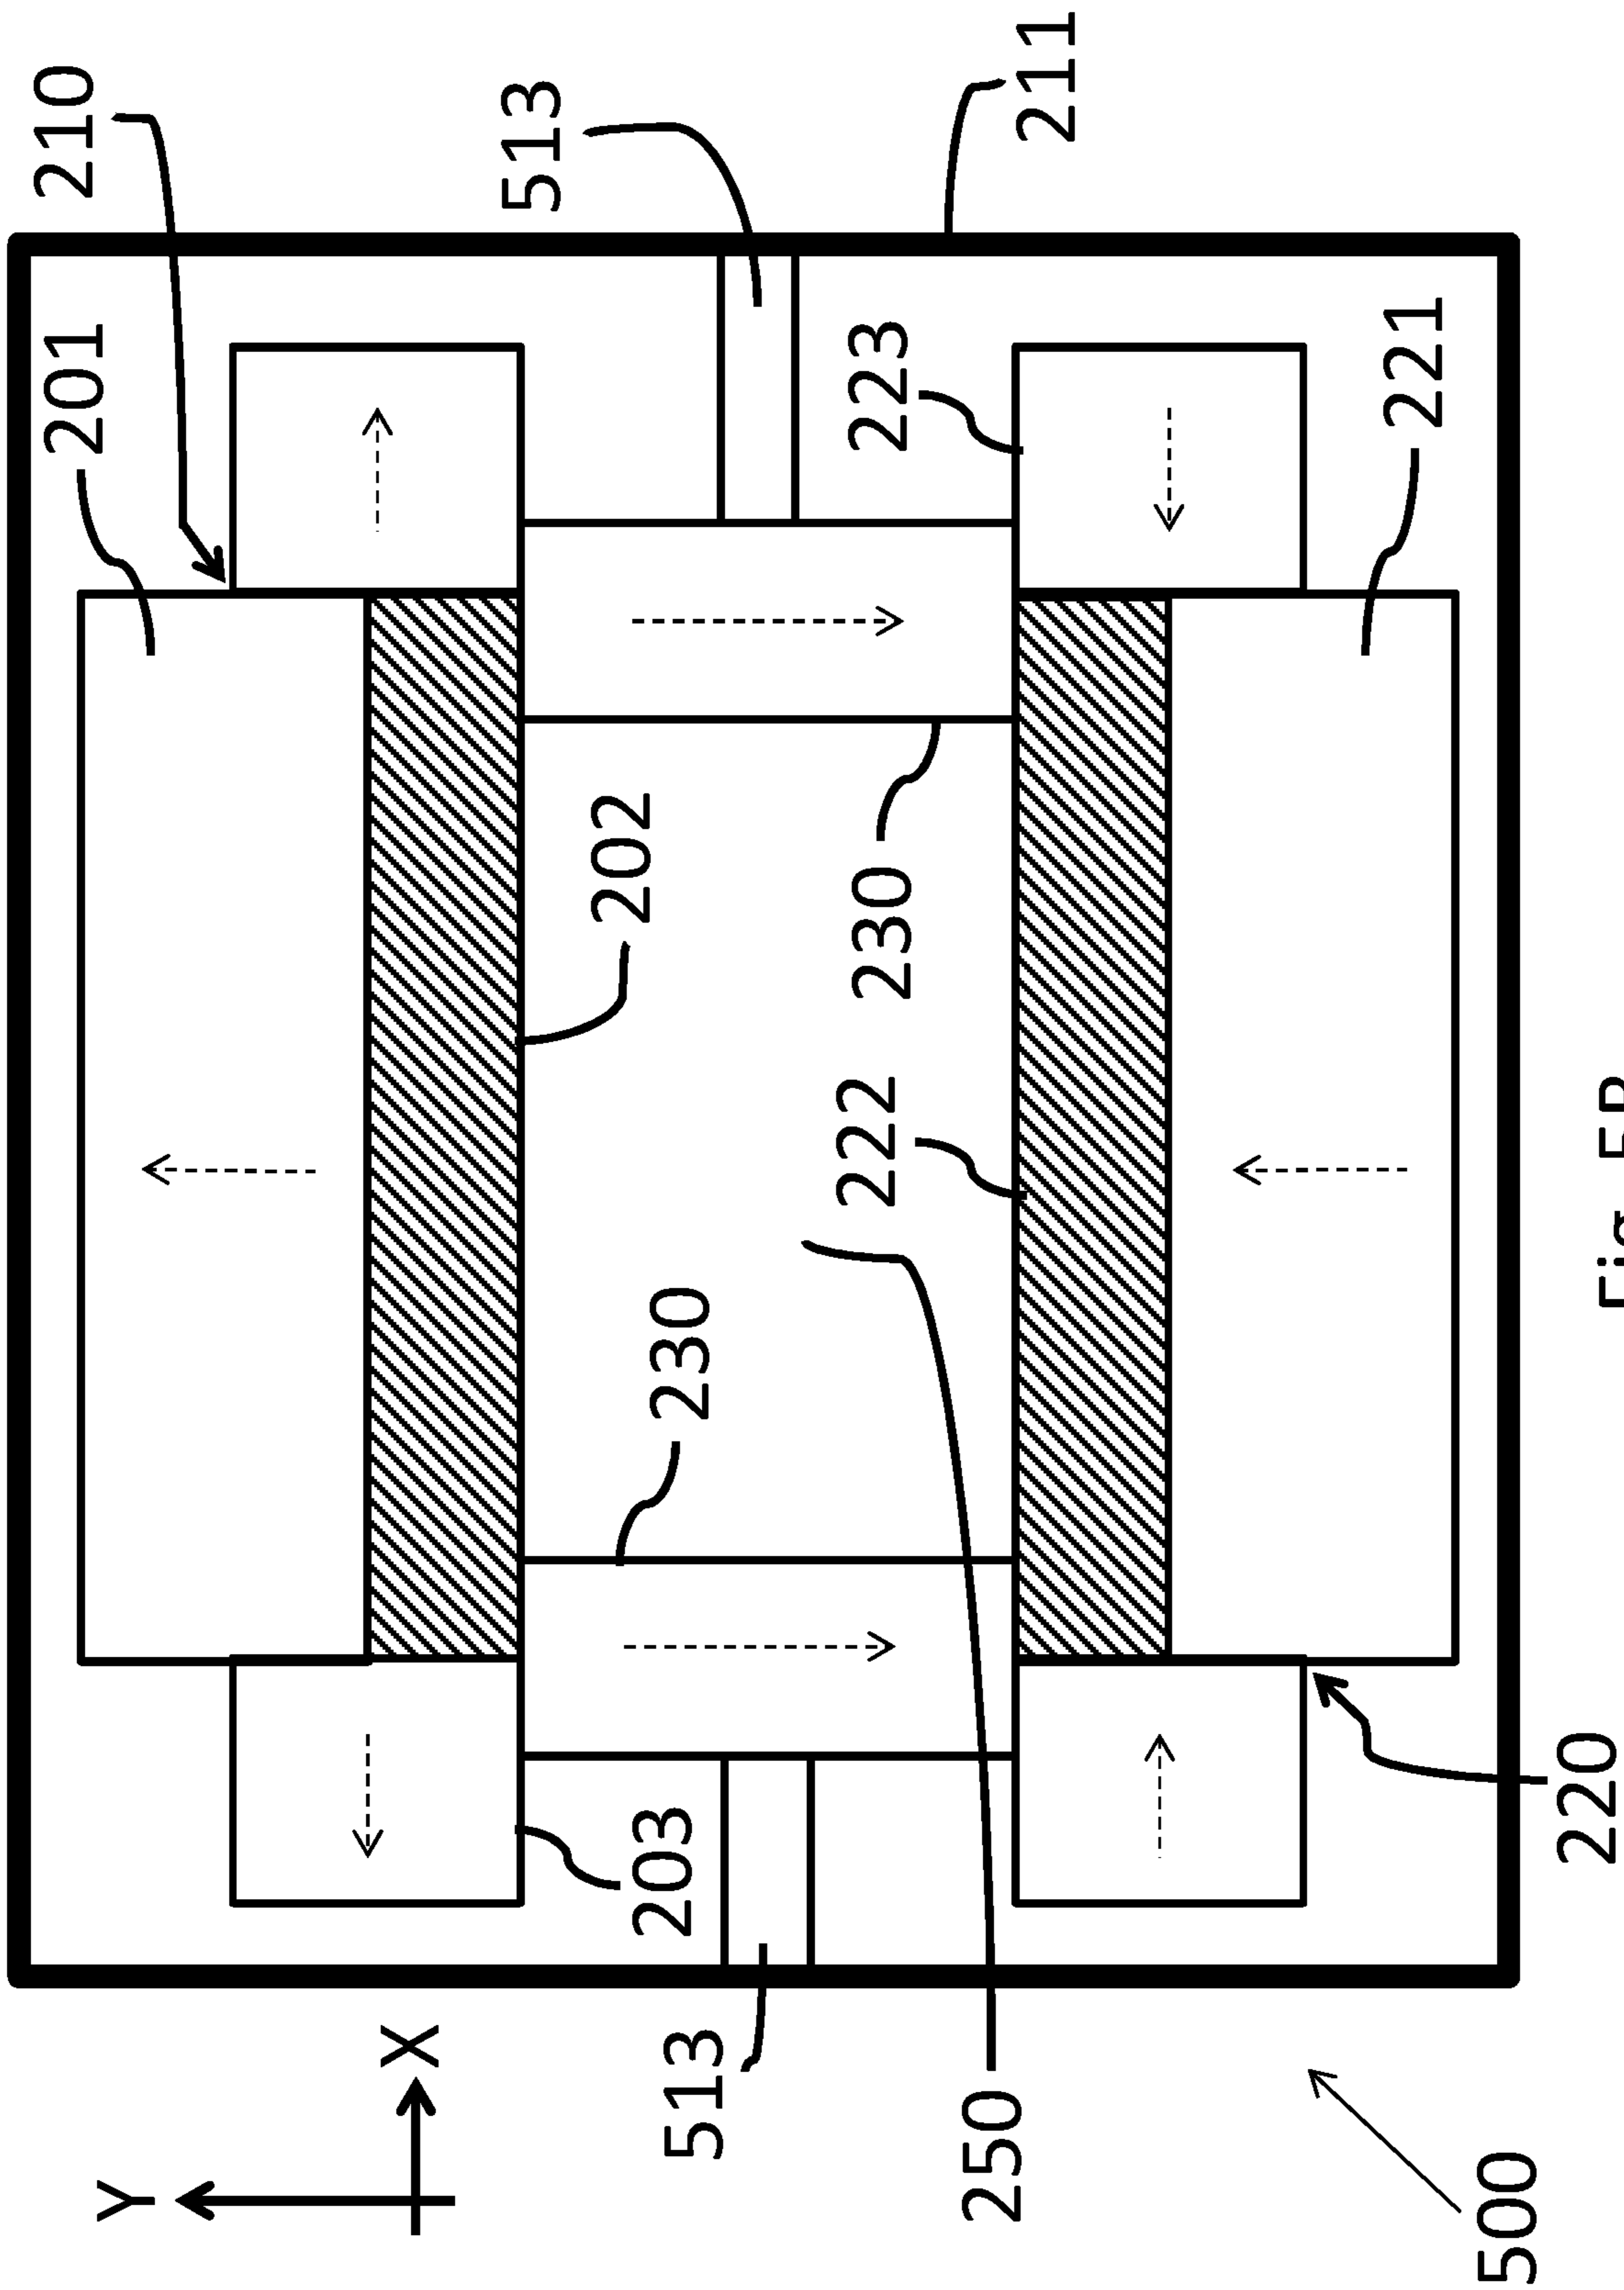


Fig. 5B

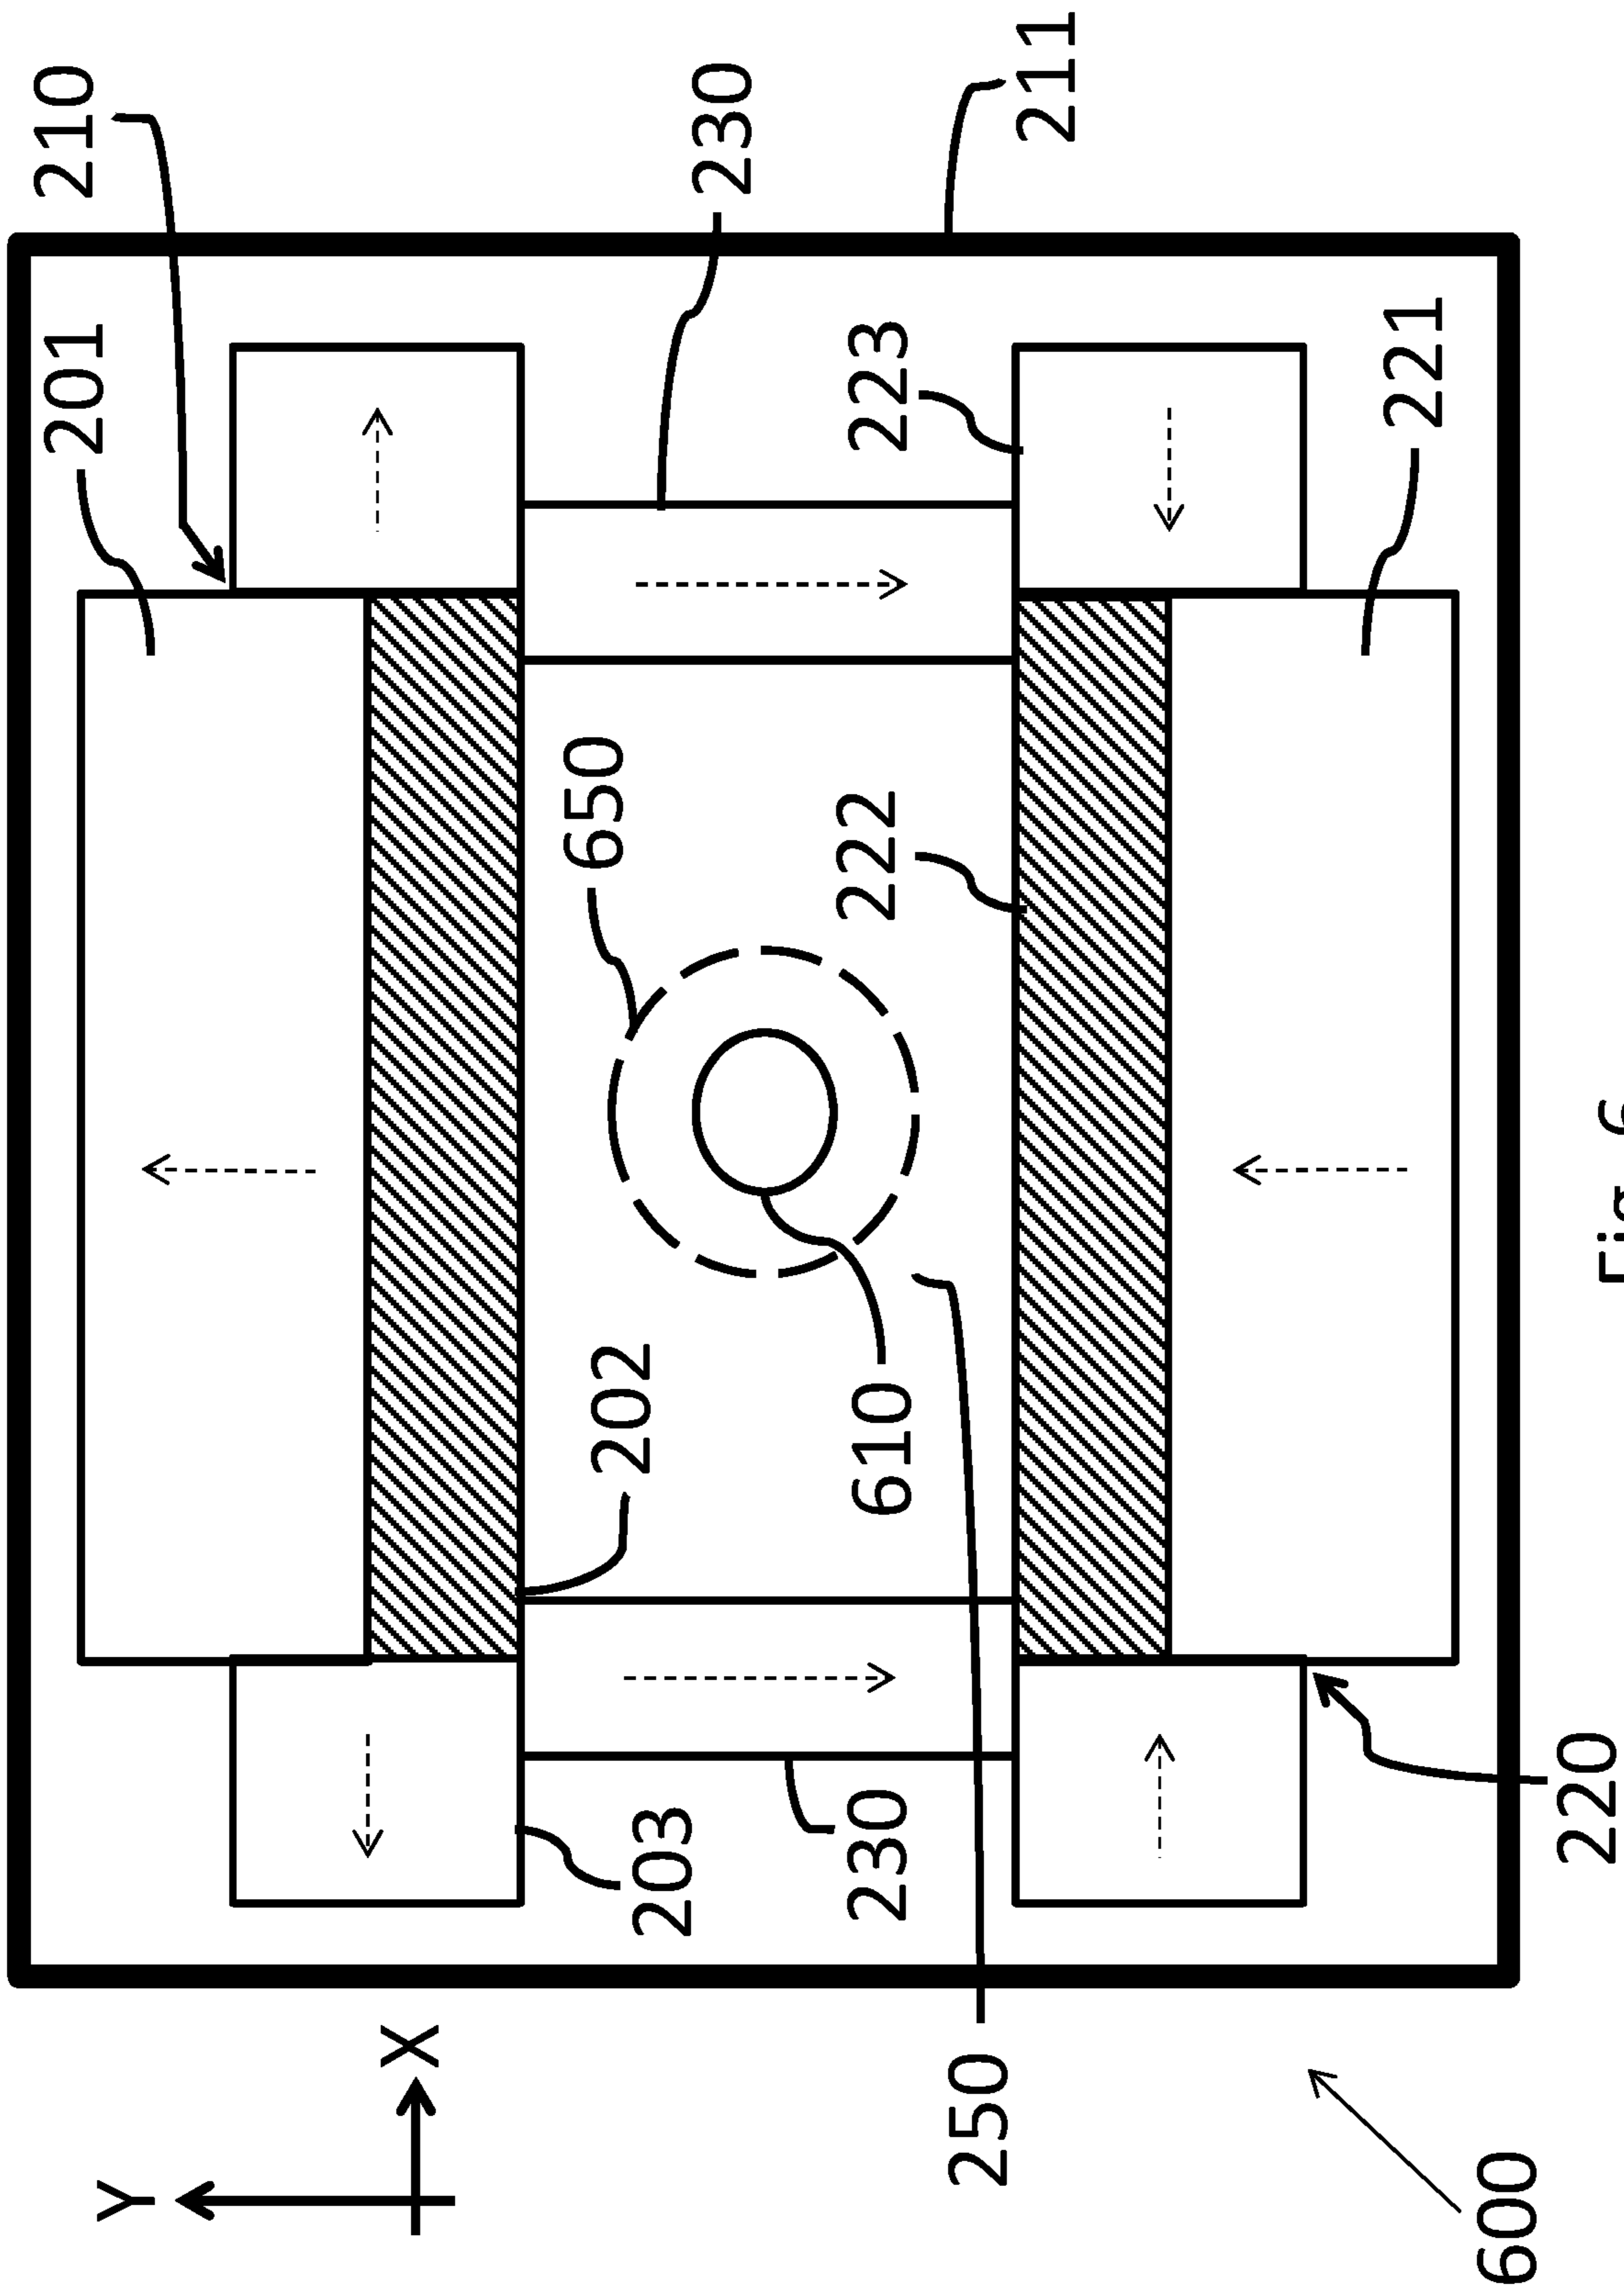


Fig. 6

1

**DEVICE, SYSTEM AND METHOD FOR  
OBTAINING A MAGNETIC MEASUREMENT  
WITH PERMANENT MAGNETS**

CROSS REFERENCE TO RELATED  
APPLICATION

This application is a continuation of U.S. patent application Ser. No. 15/402,438 filed on Jan. 10, 2017 entitled “Device, Systems and Method for Obtaining a Magnetic Measurement with Permanent Magnets,” which claims benefit of and priority to U.S. Provisional Patent Application No. 62/372,065 filed on Aug. 8, 2016 entitled “Device, Systems and Method for Obtaining a Magnetic Measurement with Permanent Magnets” and U.S. Provisional Patent Application No. 62/381,079 filed on Aug. 30, 2016 entitled “NMR/MRI Magnet Assembly Comprising Superconducting Coils and a Ferromagnetic Pole Piece,” incorporated herein by reference in their entireties.

FIELD OF THE INVENTION

Generally, the present invention relates to magnetic devices. More particularly, the present invention relates to devices, systems and methods for obtaining magnetic measurements.

BACKGROUND OF THE INVENTION

Electromagnetic based instruments can be used for measuring properties of matter and/or used for identifying its composition. For example, an electromagnetic based instrument capable of performing magnetic resonance spectroscopy can be used to obtain physical, chemical and/or structural information about matter (e.g., a molecule). Typically, in order to perform magnetic resonance spectroscopy, for example to provide high quality measurements of an object/subject (e.g., high resolution image and/or image contrast), it can be desirable for the magnetic field inside of a zone of measurement (e.g., an area where an object is to be measured is positioned) to be substantially stable and/or uniform. Other applications (e.g., magnetic resonance imaging (MRI)) can also require a high, stable, and/or uniform magnetic field strength.

Some systems that use magnetic fields for measurements can include magnetic coils to create the magnetic fields, with application of current to the coil, while other systems can utilize permanent magnets to create the magnetic fields, which typically do not require application of a current.

One difficulty in creating a magnetic field in a zone of measurement with permanent magnet(s) that is sufficient for magnetic resonance spectroscopy and/or magnetic imaging (e.g., that is substantially stable and/or uniform) is that magnetic fields produced by the permanent magnets(s) can be non-homogeneous, thus typically resulting in a non-homogenous magnetic field within the zone of measurement.

Some current solutions for creating a homogenous and/or stable magnetic field within a zone of measurement using a permanent magnet can include adding additional elements to an imaging device (e.g., coils) and/or increasing the size of the permanent magnets. One difficulty with current solutions is that as the number of elements in a magnetic measurement device increases and/or the size of the permanent magnets increases, the weight, size and/or cost of the device can increase.

2

Another difficulty with current solutions is that a magnetic measurement device that is heavy can cause a lack of mobility. For example, for magnetic measurement devices in a hospital setting (e.g., magnetic resonance imaging (MRI) devices), a heavy and/or large device can prevent hospital personnel from moving an MRI. This can cause further difficulties, when imaging patients that can be hard to move (e.g., patients that are hooked up to multiple life support and/or monitoring equipment).

In another example, for magnetic measurement devices in an industrial setting (e.g., nuclear magnetic measurement (NMR) devices that measure properties of fluids and/or drilling muds in oil production facilities), a heavy and/or large device can prevent personnel from measuring the fluids/muds at various locations in the processes.

Therefore it can be desirable to achieve a desired magnetic field strength, having sufficient homogeneity and/or stability, and/or reducing a total weight of a magnetic measurement system.

SUMMARY OF THE INVENTION

There is thus provided, in accordance with some embodiments of the invention, a magnetic field device, including a first magnet, a first ferromagnetic element positioned adjacent to the first magnet, a second magnet, a second ferromagnetic element positioned adjacent to the second magnet and relative to the first ferromagnetic element to create a gap between the first ferromagnetic element and the second ferromagnetic element, and a third magnet positioned between the first ferromagnetic element and the second ferromagnetic element and within the gap.

In some embodiments, the third magnet has a first surface that faces a first surface of the first ferromagnetic element and a second surface that faces a first surface of the second ferromagnetic element. In some embodiments, the first surface of the third magnet abuts the first surface of the first ferromagnetic element and the second surface of the third magnet abuts the first surface of the first ferromagnetic element. In some embodiments, the third magnet has a dimension that allows the third magnet to translate between a first position and a second position, the first position being the first surface of the first ferromagnetic element, the second position being the first surface of the second ferromagnetic element.

In some embodiments, the magnetic field device further includes a fourth magnet positioned between the first ferromagnetic element and the second ferromagnetic element and within the gap. In some embodiments, the fourth magnet has a first surface that faces a first surface of the first ferromagnetic element and a second surface that faces a first surface of the second ferromagnetic element. In some embodiments, the fourth magnet has a dimension that allows the fourth magnet to translate between a first position and a second position, the first position being the first surface of the first ferromagnetic element, the second position being the first surface of the second ferromagnetic element.

In some embodiments, the first magnet, the second magnet and the third magnet are permanent magnets, superconducting magnets, or resistive magnets. In some embodiments, the first magnet, the second magnet and the third magnet have dimensions that are based on a desired magnetic field strength, a type of object to be imaged, or any combination thereof. In some embodiments, the first magnet, the second magnet and the third magnet has a length



between 10 and 1100 millimeters, a width between 10 and 300 millimeters, and a height between 45 and 200 millimeters.

In some embodiments, the gap has dimensions that are based on a type of object to be imaged. In some embodiments, the gap has a diameter of 190 millimeters. In some embodiments, the magnetic field device further includes at least one fifth magnet coupled to the first magnet.

In some embodiments, the third magnet is positioned to cause a decrease of a magnetic field that is peripheral to the magnetic field device. In some embodiments, a first axis of the magnetic field device is defined as passing from the first ferromagnetic element to the second ferromagnetic element, wherein the first magnet and the second magnet are positioned to cause a magnetic field with a magnetization direction along the first axis, and wherein the third magnet is positioned to cause a magnetic field with a magnetization direction along the first axis.

In some embodiments, the magnetization direction of the third magnet is opposite of the magnetization direction of the first magnet. In some embodiments, the magnetic field device is positioned within an outer shell, the outer shell including a metal alloy. In some embodiments, at least one of the first and second magnets emits a magnetic field with a predetermined magnetic field strength, wherein the third magnet emits a magnetic field with a predetermined magnetic field strength, and wherein the strength of the magnetic field of at least one of the first and second magnets is substantially greater than the strength of the magnetic field of the third magnet. In some embodiments the total magnetic field produced during operation of the magnetic field device is substantially homogeneous and uniform within the gap

There is thus provided, in accordance with some embodiments of the invention, a method of directing magnetic fields into a measurement volume, the method including generating a first magnetic field in a first direction with a first magnetic field strength, distributing the first magnetic field into the measurement volume to create a substantially uniform magnetic flux, and increasing a total magnetic flux into the measurement volume by directing a second magnetic field in a second direction with a second magnetic field strength, wherein the second direction is parallel to the first direction.

In some embodiments, the method further includes directing a third magnetic field into the measurement volume in a third direction, wherein the third direction is perpendicular to the first direction. In some embodiments, the method further includes positioning an object within the measurement volume, and performing magnetic field analysis on the object.

In some embodiments, at least one of the first magnetic field strength, and the second magnetic field strength is between 0.5 and 1.5 Tesla. In some embodiments, the first magnetic field strength and the first direction, and the second magnetic field strength and the second direction are based on a size of the measurement volume, a type of object to be measured, or any combination thereof. In some embodiments, the total magnetic flux in the measurement volume is a substantially homogeneous field.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The subject matter regarded as the invention is particularly pointed out and distinctly claimed in the concluding portion of the specification. The invention, however, both as to organization and method of operation, together with objects, features, and advantages thereof, can be understood

by reference to the following detailed description when read with the accompanying drawings in which:

FIG. 1A schematically illustrates a perspective cross-sectional view of a magnetic field device, according to illustrative embodiments of the invention;

FIG. 1B schematically illustrates a perspective cross-sectional view of a magnetic field device having additional magnets to the device of FIG. 1A, according to illustrative embodiments of the invention;

FIG. 2A schematically illustrates a frontal cross-sectional view of the magnetic field device, according to illustrative embodiments of the invention;

FIG. 2B schematically illustrates a frontal cross-sectional view of the magnetic field device, with additional magnets, according to illustrative embodiments of the invention

FIG. 3 shows a flow chart for a method of directing magnetic fields into a measurement volume, according to illustrative embodiments of the invention;

FIGS. 4A-4H schematically illustrate top cross-sectional views of various magnetic field devices, according to illustrative embodiments of the invention;

FIG. 5A schematically illustrates a frontal cross-sectional view of a magnetic field device, according to illustrative embodiments of the invention;

FIG. 5B schematically illustrates a frontal cross-sectional view of a magnetic field device, according to illustrative embodiments of the invention; and

FIG. 6 schematically illustrates a frontal cross-sectional view of a head magnetic field device, according to illustrative embodiments of the invention.

It will be appreciated that for simplicity and clarity of illustration, elements shown in the figures have not necessarily been drawn to scale. For example, the dimensions of some of the elements can be exaggerated relative to other elements for clarity. Further, where considered appropriate, reference numerals can be repeated among the figures to indicate corresponding or analogous elements.

#### DETAILED DESCRIPTION OF THE INVENTION

In the following detailed description, numerous specific details are set forth in order to provide a thorough understanding of the invention. However, it will be understood by those skilled in the art that the present invention can be practiced without these specific details. In other instances, well-known methods, procedures, and components have not been described in detail so as not to obscure the present invention.

FIG. 1A schematically illustrates a cross-sectional perspective view of a magnetic field device **100**, according to illustrative embodiments of the invention. The magnetic field device **100** can include an outer shell **111**, a first magnet **101** (e.g., a first permanent magnet), a first ferromagnetic element **102** (e.g., a first pole piece), and a second magnet **121** (e.g., a second permanent magnet) and a second ferromagnetic element **122** (e.g., a second pole piece). In some embodiments, first magnet **101** and first ferromagnetic element **102** and/or second magnet **121** and second ferromagnetic element **122** can be grouped together as a single unit (e.g., as an assembly).

The first ferromagnetic element **102** can be coupled to and/or positioned adjacent to the first magnet **101**. The second ferromagnetic element **122** can be coupled to and/or positioned adjacent to the second magnet **121**. In some embodiments, the magnetic field device **100** can include a

third magnet **130**, positioned between the first ferromagnetic element **102** and the second ferromagnetic element **122**.

The first and second ferromagnetic elements **102**, **122** can be coupled and positioned adjacent to a corresponding first and second magnets **101**, **121** such that the first and second ferromagnetic elements **102**, **122** can be proximal to a gap **150** (e.g., zone of measurement) of the magnetic field device **100**. The first magnet **101** and the second magnet **121** can be distal to the gap **150** of the magnetic field device **100**. The magnetization direction of the first magnet **101** can be parallel to the magnetization direction of the second magnet **121**, along the second axis (indicated "X" in FIG. 1A), where the first and second ferromagnetic elements **102**, **122** can face each other with the gap **150** created therebetween.

In various embodiments, dimensions of the gap **150** (and thus positioning on of the elements **102**, **122**, **101**, **121**) can depend on a subject/object to be measured. For example, if the subject to be measured is an adult human head gap **150** can have dimensions that comfortably fit an adult human head. In another example, if the subject to be measured is a mouse, gap **150** can fit the mouse. It is apparent to one of ordinary skill that other objects/subjects can be measured, and that these are examples.

FIG. 1B schematically illustrates a cross-sectional perspective view of a magnetic field device **200**, having additional magnets to the device of FIG. 1A, according to illustrative embodiments of the invention. The magnetic field device **200** can include an outer shell **211**, a first magnet **201**, a first ferromagnetic element **202** (e.g., a first pole piece), a second magnet **221**, a third magnet **230**, a fourth magnet **240**, a first ferromagnetic element **202**, and a second ferromagnetic element **222** (e.g., a second pole piece). The first ferromagnetic element **202** can be coupled to and/or positioned adjacent to the first magnet **201**. The second ferromagnetic element **222** can be coupled to and/or positioned adjacent to the second magnet **221**.

In some embodiments, the magnetic field device **200** can include additional magnets such as magnets **103**, **123** in FIG. 1A or magnets **203**, **223** in FIG. 1B. In some embodiments, magnets **103**, **123** in FIG. 1A are not present.

The first and second ferromagnetic elements **202**, **222** can be coupled to and positioned adjacent to its corresponding first and second magnets **201**, **221** such that the first and second ferromagnetic elements **202**, **222** can be proximal to a gap **250** (e.g., zone of measurement) of the magnetic field device **200**. The first magnet **201** and the second magnet **221** can be distal to the gap **250** of the magnetic field device **200**. The magnetization direction of the first magnet **201** can be parallel to the magnetization direction of the second magnet **221**, along the second axis (indicated "X" in FIG. 1B), where the first and second ferromagnetic elements **202**, **222** can face each other with the gap **250** created therebetween.

The third magnet **230** can be coupled to and can be positioned between the first ferromagnetic element **202** and the second ferromagnetic element **222**.

The third magnet **230** can have a first surface **231** that faces a first surface **204** of the first ferromagnetic element **202** and a second surface **232** that faces a first surface **224** of the second ferromagnetic element **222**. The first surface **231** of the third magnet **230** can abut the first surface **204** of the first ferromagnetic element **202** and the second surface **232** of the third magnet **230** can abut the first surface **224** of the second ferromagnetic element **222**. In some embodiments, the third magnet **230** can have a dimension that allows the third magnet **230** to translate between a first position and a second position, the first position being the

first surface **204** of the first ferromagnetic element **202**, the second position being the first surface **224** of the second ferromagnetic element **222**.

The fourth magnet **240** can be positioned between the first ferromagnetic element **202** and the second ferromagnetic element **222** and within the gap **250**. The fourth magnet **240** can have a first surface **241** that faces the first surface **204** of the first ferromagnetic element **202** and a second surface **242** that faces the first surface **224** of the second ferromagnetic element **222**. The fourth magnet **240** can have a dimension that allows the fourth magnet **240** to translate between a first position and a second position, the first position being the first surface **204** of the first ferromagnetic element **202**, the second position being the first surface **224** of the second ferromagnetic element **222**.

As is apparent to one of ordinary skill in the art, while magnetic gradient coils (creating a magnetic field with application of current) can be utilized in the gap to provide a magnetic gradient, an embodiment of the invention uses permanent magnets that have no need for magnetic gradient coils.

In some embodiments, the first magnet **201**, the second magnet **221** and the third magnet **230** are permanent magnets and/or superconducting magnets and/or resistive magnets. The first magnet **201**, the second magnet **221** and the third magnet **230** can have dimensions that are based on a desired magnetic field strength, a type of object to be imaged, or any combination thereof.

In some embodiments, at least one of the first magnet **201**, the second magnet **221** and the third magnet **230** has a length between 10 and 1100 millimeters, a width between 10 and 300 millimeters, and a height between 45 and 200 millimeters.

Each of the magnets of magnetic field device **200** has a direction of magnetization and creates a magnetic field. The dashed arrows in FIG. 1B indicate a direction of the magnetization of the particular magnet the arrow is displayed on.

The first magnet **201** and second magnet **221** can have the same magnetization direction along a first axis (indicated "Y" in FIG. 1B), for example a transverse axis of the magnetic field device **200**.

The magnetization direction of the third magnet **230** can be opposite to the magnetization direction of the first and second magnets **201**, **221** for instance along the first axis (indicated "Y" in FIG. 1B).

In some embodiments, the first ferromagnetic element **202** and the second ferromagnetic element **222** can extend and can direct the magnetic field produced by the corresponding first magnet **201** and second magnet **221**, and/or reduce noise from outside of the magnetic field device **200**.

FIG. 2A schematically illustrates a frontal cross-sectional view of the magnetic field device **200**, according to illustrative embodiments of the invention. FIG. 2B schematically illustrates a frontal cross-sectional view of the magnetic field device **200**, with additional magnets, according to illustrative embodiments of the invention.

In some embodiments, the magnetic field device **200** can include additional magnets. For example, turning to FIG. 2B, the magnetic field device **200** can include a fifth magnet **203**, and a sixth magnet **223**. In some embodiments, at least one of fifth magnet **203** and sixth magnet **223** is a permanent magnet.

In some embodiments, the magnetic field device **200** can include additional magnets **203**, **223** while the third magnet **230** can be coupled to the first and second ferromagnetic elements **202**, **222**.

In various embodiments, the fifth and sixth magnets **203**, **223** are positioned around the first and second magnets **201**, **221**, respectively, for instance the sixth magnet **223** can be positioned around the second magnet **221**.

The fifth and sixth magnets **203**, **223** can have a magnetization direction perpendicular to the magnetization direction of the first magnets **201** along a second axis (indicated "X" in FIG. 2B) perpendicular to the first axis, for example a longitudinal axis of the magnetic field device **200**. According to some embodiments, the magnetization direction of the at least one fifth magnet **203** can be away from the first magnet **201**, and the magnetization direction of the at least one sixth magnet **223** can be towards the second magnet **221**.

As is apparent to one of ordinary skill in the art, additional magnets can be included in the magnetic field device **200**. For example, in some embodiments, additional third magnets, fifth magnets and/or first magnets can be used.

In some embodiments, the outer shell **211** can include a metal alloy, and can allow confining (or substantially confining) the magnetic field created by the magnets of magnetic field device **200** within the outer shell **211**. In this manner, the existence of a magnetic field outside of the outer shell **211** can be zero and/or negligible. For example, if a device that is susceptible to the effects of a magnetic field (e.g., cell phone, pacemaker, etc.) is positioned adjacent to the outer shell **211** outside of the device **200**, the magnetic field in that location can have a negligible effect on the device. In some embodiments, outer shell **211** can also have an opening so as to provide access to the gap **250**.

In various embodiments, the third magnet **230** and/or the fourth magnet **240** can have a hollow structure and surround the gap **250** between the first and second ferromagnetic elements **202**, **222**. In various embodiments, the third magnet **230** and/or the fourth magnet **240** can be provided in a variety of shapes and sized, for instance cylindrical or triangular, with varying shape and size.

In case that magnetic field device **200** is utilized for magnetic resonant imaging, additional electromagnetic elements can be included, such as a radio frequency (RF) generator or field sensors. The third magnet **230** can be configured to surround the gap **250** between the first and second ferromagnetic elements **202**, **222** in order to for example, prevent radiation leakage from additional electromagnetic elements, for instance RF generator in magnetic resonance devices. For example, third magnet **230** can be in a shape of a hollow cube or a hollow cylinder surrounding gap **250** in order to, for example, prevent radiation leakage from additional electromagnetic elements outside of third magnet **230**.

The third magnet **230** can contribute to causing the overall magnetic field to be a homogeneous and/or uniform magnetic field, for magnetic field device **200** in the area of measurement. The third magnet **230** can allow for a reduction of size, weight, and/or magnetic field strength of the first and/or second magnets **201**, **221** and/or the fifth and/or sixth magnets **203**, **223** due to, for example, the third magnet **230** contributing to the overall magnetic field strength within the gap. A reduction in size of the first and/or second magnets **201**, **221** and/or the fifth and/or sixth magnets **203**, **223**, can allow for a having lower weight of the magnetic field device with substantially the same field strength compared to, for example, a magnetic field device that does not include the third magnet **230**.

In some embodiments, magnetic field device **200** includes two fifth magnets **203**, and also includes two sixth magnets **223**. In these embodiments, the ability to reduce the size of

the magnets due to, for example, the third magnet **230** can provide even further weight reduction of the magnetic field device.

In some embodiments, at least one of the first and second magnets **201**, **221** emits a magnetic field with a predetermined magnetic field strength, wherein the third magnet **230** can emit a magnetic field with a predetermined magnetic field strength, and wherein the strength of the magnetic field of at least one of the first and second magnets **201**, **221** can be substantially greater than the strength of the magnetic field of the third magnet **230**.

According to some embodiments, the outer shell **211** can constitute the main bulk of the weight of the magnetic field device **200**. Since the addition of the third magnet **230** can reduce weight of other components as well as provide a homogeneous and uniform magnetic field, it can be possible to utilize an outer shell with reduced weight. In some embodiments, a reduction of at least twenty percent can be created for the total weight of the magnetic field device **200** in comparison to, for example, devices that do not have the third magnet. In some embodiments, an increase of at least thirty percent can be created for the magnetic field strength, for example in comparison to, for example, device that do not have the third magnet but have substantially the same total weight of the magnetic field device **200**. The third magnet **230** can allow obtaining stronger magnetic fields and/or lower total magnet weight.

In some embodiments, the area of the fringe field can be reduced from the center of the gap, for example for a limit of a field of about 1 Gauss (sometimes referred to as the 1G line) can be reduced at substantially 100 millimeters. Therefore, reduction of fringe field can cause the dimensions of the outer shell **211** to be reduced, for example, from substantially 860×1032 millimeters to substantially 786×894 millimeters. Reduction of the outer shell **211** can accordingly cause a reduction of the total weight of magnetic field device **200**.

Overall weight of a magnetic field device can be reduced, and for example an increase of over ten percent for the ratio of magnetic field strength to total weight of at least the combination of the first and second magnets and the at least one third magnet. In some embodiments, an increase in magnetic field caused by the third magnets can be larger than the increase that may be achieved by a corresponding enlargement of the first and second magnets (without a third magnet). This is due to the alignment of the third permanent magnets and also due to the scalability of the weight savings such that addition of magnets can cause a reduction of weight.

In some embodiments, the outer shell **211** can also have a smaller surface area compared to a commercially available magnetic resonance device, due to a reduction in fringe weight of the outer shell and/or due to reduction of the fringe field. Such reduction can occur since the addition of the third magnet **230** can increase magnetic field in the gap **250**, between the first and second ferromagnetic elements **202**, **222** and therefore reduce the fringe field of the magnetic field device **200** so that there is no longer a need for the outer shell **211** to be at same large weight and large surface area, for example compared to a commercially available magnetic resonance device.

In some embodiments, additional material, for example including Iron, can be added to magnetic field device **200** in order to further confine and manipulate the magnetic field in the gap. In some embodiments, the added material, for example including Iron and/or Titanium, can be added

adjacent to at least one magnet **201** and/or adjacent to at least one ferromagnetic element **202**.

It may be appreciated that regions of high magnetic flux density causing external fringe fields can occur adjacent to connection of the magnets, e.g., indicated with a dashed line in FIG. 4A. In some embodiments, an outer shell (or envelope), usually including Iron, surrounds the magnetic resonance device to reduce the magnetic flux.

In some embodiments, the third magnet **230** can prevent at least a portion of magnetic flux from exiting a gap (e.g., an area where the magnetic field is directed). Magnetic field device **200** can be utilized in order to provide a strong magnetic field while providing reduced weight of the device, for example utilized for magnetic resonant imaging or for other devices where a strong magnetic field can be required. It may be appreciated that addition of the third magnets can counter the magnetic flux, for example in regions indicated with a dashed line in FIG. 4A, so as to, for example, reduce the fringe fields.

According to some embodiments, an existing magnetic field system that includes two magnets, neither of which includes a third magnet can be modified with insertion of at least one third magnet between the two magnets, in order to, for example, increase the magnetic field within the gap and/or reduce the fringe field. For example, a comparison between three systems: a first system "A" without third magnets, a second system "B" provided with at least one third magnet, and a third system "C" that is modified with the addition of at least one third magnet. In this example, in weight comparison to the first system "A", the second system "B" can have weight reduced at about 5.5%, while the third system "C" can have weight increase at about 6.5%. In this example, in comparison to the first system "A" of field strength in the gap, the second system "B" can have increase of about 15%, and the third system "C" can have increase of about 13%. In this example, in comparison to the first system "A" of fringe field reduction, the second system "B" can have decrease of about 55%, and the third system "C" can have decrease of about 16%. Therefore, in correct positioning of third magnets can provide various advantages to new systems as well as to existing systems that can be modified. It is apparent to one of ordinary skill in the art that the example provided above gives exemplary weight reduction values for explanatory purposes, and that other comparison weight configurations are within the scope of the invention.

Reference is now made to FIG. 3, which shows a flow chart for a method of directing magnetic fields into a measurement volume, according to some embodiments of the invention.

The method includes generating a first magnetic field in a first direction with a first magnetic field strength (Step 301). For example, the first and second magnets **201** and **221** as described above in FIG. 1B can direct a first magnetic field in a first direction and having first magnetic field strength.

The method can further include distributing the first magnetic field into the measurement volume to create a substantially uniform magnetic flux. (Step 302). For example, the first ferromagnetic element **202** and/or the second ferromagnetic element **222**, as described above in FIG. 1B can distribute the first magnetic field into the measurement volume.

The method can further include increasing a total magnetic flux into the measurement volume by directing a second magnetic field in a second direction with a second magnetic field strength, where the second direction is parallel to the first direction (Step 303). For example, the third

magnet **230** as described above in FIG. 1 can direct a second magnetic field in a second direction and having second magnetic field strength. In some embodiments, the method includes directing a third magnetic field in a third direction having a third magnetic field strength, wherein the third direction is perpendicular to the first direction. For example, the fifth magnets **203** and/or sixth magnets **223** as described above in FIG. 2 can direct a third magnetic field in a third direction and having third magnetic field strength.

In some embodiments, the method includes positioning an object within the measurement volume, and performing magnetic field analysis on the object (e.g., by using the magnetic device **200** within a NMR device and/or an MRI device).

In some embodiments, first, second and third magnetic fields are directed such that a desired magnetic field strength is achieved. The desired magnetic field strength can be based on a particular device performing the measurements and/or object to be measured. For example, the desired magnetic field strength can be between 0.5-1.5 T, for magnetic resonance imaging of living human tissue. As is apparent to one of ordinary skill in the art, the desired magnetic field strength shown is for exemplary purposes only, and that the desired magnetic field strengths can vary based on subject/application of the magnetic field.

In some embodiments, the first magnetic field strength and the first direction, and the second magnetic field strength and the second direction are based on a size of the measurement volume and/or type of object to be measured, and/or any combination thereof. In some embodiments, the total magnetic flux in the measurement volume can be a substantially homogeneous field.

Reference is now made to FIGS. 4A-4H, which schematically illustrate a top cross-sectional view of some exemplary configurations for magnetic components of a magnetic field device (for example magnetic field device **200**), according to some embodiments of the invention. FIG. 4A schematically illustrates a first exemplary configuration, where at least one third magnet **430** (similar to the third magnet **230**, as shown in FIGS. 1-2) can be positioned adjacent to the first magnet **401** (similar to the first magnet **201**, as shown in FIGS. 1-2), for example perpendicularly. Such positioning can be utilized to at least partially surround and/or envelope the gap **450** (similar to gap **250**, as shown in FIGS. 1-2). In some embodiments, a plurality of the third magnets **430** can be utilized, wherein each third magnet **430** (e.g., main magnets) can have a different size and/or shape. In some embodiments, the fifth and sixth magnets can be positioned such that they do not physically contact the third magnets.

FIG. 4B schematically illustrates a first exemplary configuration, where at least one first intermediate magnet **432** (e.g., main magnet) can be positioned between two adjacent third magnets **430**. FIG. 4C schematically illustrates a first exemplary configuration, where at least one second intermediate magnet **434** e.g., main magnet) can be positioned between adjacent third magnet **430** and first intermediate magnet **432**. In some embodiments, at least one of first intermediate magnet **432** and/or second intermediate magnet **434** can be a permanent magnet.

According to some embodiments, an object (or a subject) can be introduced to the gap (or measurement region), for example in order to adjust an element therein, from any one of four possible directions due to, for example, the symmetry of the system. In some embodiments, access can also be provided for introduction of cameras, air conditioning and/or other equipment to be adjacent to the gap.

FIG. 4D schematically illustrates a first exemplary configuration, where at least one first intermediate magnet 442 can be positioned between two adjacent third magnets 440 and at least one second intermediate magnet 444 can be positioned between two adjacent third magnets 440. Different sizes and/or shapes of at least one first intermediate magnet 442 and at least one second intermediate magnet 444 can allow differentiation of the magnets, e.g., providing smaller magnets of different shapes at particular locations instead of single large magnet, in order to allow a desired magnetic flux within the gap 450. In case that shape symmetry about an axis through the center of the third magnet is broken, e.g., for magnetic shimming and/or for creation of an opening to allow access to the gap, other elements (e.g., permanent magnets) can be modified so as to maintain the predetermined magnetic field. In some embodiments, a break in symmetry, e.g., of the shape of the magnet, can require modification of the outer shell as well.

FIG. 4E schematically illustrates a first exemplary configuration, where at least one first intermediate magnet 442 can be positioned at a predetermined distance, based on the predetermined magnetic field strength, from the center of first magnet 401, in order to allow a desired magnetic flux within the gap 450. FIG. 4F schematically illustrates a first exemplary configuration, where at least one first intermediate magnet 442 can be positioned between two adjacent third magnets 440 and at least one second intermediate magnet 444 can be positioned between two adjacent third magnets 440. In some embodiments, addition of the at least one first intermediate magnet 442 can be configured to further support the structure of the system and/or to create at least a partial magnetic cage within the gap 450.

FIG. 4G schematically illustrates a first exemplary configuration, where a circularly shaped third magnet 460 can surround the gap 450. FIG. 4H schematically illustrates a first exemplary configuration, where a hexagon shaped third magnet 470 can surround the gap 450. In some embodiments, an opening can be provided in a third magnet surrounding the gap 450 in order to allow insertion of an object therein.

Reference is now made to FIGS. 5A-5B, which show the magnetic field device 500 (e.g., magnetic field device 200 as described above in FIG. 2) including support elements. FIG. 5A schematically illustrates a frontal cross-sectional view of a magnetic field device 500 having first support elements 511, according to some embodiments of the invention. It may be appreciated that the magnetic field device 500 can include all elements of the magnetic field device 200 (e.g., as shown in FIGS. 1-2) with the addition of at least one first support element 511 between the first ferromagnetic element 202 and the second ferromagnetic element 222.

According to some embodiments, at least one third magnet 530 can be added to a first support element 511 such that at least one air gap (not shown) can be created between the third magnet 530 and the first and/or second magnets 201, 221. In some embodiments, instead of air gaps, a gap of diamagnetic material can be formed therein.

FIG. 5B schematically illustrates a frontal cross-sectional view of a magnetic field device 500 having second support elements 513, according to some embodiments of the invention. It may be appreciated that the magnetic field device 500 can include all elements of the magnetic field device 200 (e.g., as shown in FIGS. 1-2) with the addition of at least one second support element 513. In some embodiments, the outer shell 211 (or envelope) can contact at least one third magnet 230 with at least one second support element 513 in order to support the positioning of the third magnets 230. It

may be appreciated that such support of third magnets 230 can counter magnetic attraction forces acting on third magnets 230, such that third magnet 230 can remain in the desired position. In some embodiments, the at least one second support element 513 can couple the third magnets 230 with at least one of the outer shell 211 and first and second ferromagnetic elements 202, 222.

Reference is now made to FIG. 6, which schematically illustrates a frontal cross-sectional view of a head magnetic field device 600, according to some embodiments of the invention. The head magnetic field device 600 includes a first magnet 201 and a first ferromagnetic element 202 coupled to the first magnet 201, and a second magnet 221 and a second ferromagnetic element 222 coupled to the second magnet 221. The first magnet 201 and the second magnet 221 can be positioned to create a gap 250 therebetween, with the first ferromagnetic element 202 and the second ferromagnetic element 222 positioned adjacent the gap 250 and between the gap 250 and a respective first magnet 201 and second magnet 221. The head magnetic field device 600 can also include an opening 650, the opening configured to allow, for example, at least partial accommodation of a head 610 of a patient within the gap 250 (or measurement volume). In some embodiments, head magnetic field device 600 can also include at least one third magnet 230. It may be appreciated that while the head 610 of the patient is described here, any other body part can be similarly introduced to the gap 250 for inspection, for example and arm or a leg.

In some embodiments, magnetic resonance imaging elements (e.g., RF coil) can be coupled to the head magnetic field device 600 in order to allow imaging the head 610 of the patient within the gap 250. In an exemplary embodiment, the magnetic field strength for such a head magnet is above 4900 Gauss or about 4988 Gauss. In an exemplary embodiment, the field of view for MRI imaging within the gap 250 is a sphere with a diameter of about 190 millimeters. In an exemplary embodiment, the diameter of the opening 650 to the gap 250 is above 660 millimeters or about 665 millimeters. In an exemplary embodiment, the dimensions for a permanent head magnet are 1226×1226×866 millimeters.

Unless explicitly stated, the method embodiments described herein are not constrained to a particular order in time or chronological sequence. Additionally, some of the described method elements can be skipped, or they can be repeated, during a sequence of operations of a method.

Various embodiments have been presented. Each of these embodiments can of course include features from other embodiments presented, and embodiments not specifically described can include various features described herein.

The invention claimed is:

1. A magnetic field device, comprising:

- a first magnet;
- a first ferromagnetic element positioned adjacent to the first magnet;
- a second magnet;
- a second ferromagnetic element positioned adjacent to the second magnet and relative to the first ferromagnetic element to create a gap between the first ferromagnetic element and the second ferromagnetic element; and
- a third magnet positioned between the first ferromagnetic element and the second ferromagnetic element and within the gap; and

wherein at least one of the first and second magnets emits a magnetic field with a predetermined magnetic field strength, wherein the third magnet emits a magnetic field with a predetermined magnetic field strength, and

## 13

wherein the strength of the magnetic field of at least one of the first and second magnets is greater than the strength of the magnetic field of the third magnet.

2. The magnetic field device of claim 1, wherein the third magnet has a first surface that faces a first surface of the first ferromagnetic element and a second surface that faces a first surface of the second ferromagnetic element.

3. The magnetic field device of claim 2, wherein the first surface of the third magnet abuts the first surface of the first ferromagnetic element and the second surface of the third magnet abuts the first surface of the second ferromagnetic element.

4. The magnetic field device of claim 2, wherein the third magnet has a dimension that allows the third magnet to translate between a first position and a second position, the first position being the first surface of the first ferromagnetic element, the second position being the first surface of the second ferromagnetic element.

5. The magnetic field device of claim 1, wherein the first magnet, the second magnet and the third magnet are permanent magnets, superconducting magnets, or resistive magnets.

6. The magnetic field device of claim 1, wherein the first magnet, the second magnet and the third magnet have dimensions that are based on a desired magnetic field strength, a type of object to be imaged, or any combination thereof.

7. The magnetic field device of claim 1, wherein the gap has dimensions that are based on a type of object to be imaged.

8. The magnetic field device of claim 1, wherein the gap has a diameter of 190 millimeters.

9. The device of claim 1, wherein the third magnet is positioned to cause a decrease of a magnetic field that is peripheral to the magnetic field device.

10. The device of claim 1, wherein a first axis of the magnetic field device is defined as passing from the first ferromagnetic element to the second ferromagnetic element, wherein the first magnet and the second magnet are positioned to cause a magnetic field with a magnetization direction along the first axis, and wherein the third magnet is positioned to cause a magnetic field with a magnetization direction along the first axis.

11. The device of claim 10, wherein the magnetization direction of the third magnet is opposite of the magnetization direction of the first magnet.

12. The device of claim 1, wherein the magnetic field device is positioned within an outer shell, the outer shell comprising a metal alloy.

13. The device of claim 1, wherein the strength of the magnetic field of at least one of the first and second magnets is substantially greater than the strength of the magnetic field of the third magnet.

## 14

14. The device of claim 1, wherein the total magnetic field produced during operation of the magnetic field device is substantially homogeneous and uniform within the gap.

15. A method of directing magnetic fields into a measurement volume, the method comprising:

generating a first magnetic field in a first direction with a first magnetic field strength;

distributing the first magnetic field into the measurement volume to create a substantially uniform magnetic flux; and

increasing a total magnetic flux into the measurement volume by directing a second magnetic field into the measurement volume in a second direction with a second magnetic field strength, wherein the second direction is parallel to the first direction.

16. The method of claim 15, further comprising directing a third magnetic field into the measurement volume in a third direction, wherein the third direction is perpendicular to the first direction.

17. The method of claim 15, further comprising:

positioning an object within the measurement volume; and

performing magnetic field analysis on the object.

18. The method of claim 15, wherein at least one of the first magnetic field strength, and the second magnetic field strength is between 0.5 and 1.5 Tesla.

19. The method of claim 15, wherein the first magnetic field strength and the first direction, and the second magnetic field strength and the second direction are based on a size of the measurement volume, a type of object to be measured, or any combination thereof.

20. The method of claim 15, wherein the total magnetic flux in the measurement volume is a substantially homogeneous field.

21. A method of directing magnetic fields into a measurement volume, the method comprising:

generating a first magnetic field in a first direction with a first magnetic field strength;

distributing the first magnetic field into the measurement volume to create a substantially uniform magnetic flux;

increasing a total magnetic flux into the measurement volume by directing a second magnetic field in a second direction with a second magnetic field strength, wherein the second direction is parallel to the first direction; and

directing a third magnetic field into the measurement volume in a third direction, wherein the third direction is perpendicular to the first direction.

\* \* \* \* \*