

US010898324B2

(12) **United States Patent**  
**Morrissey et al.**

(10) **Patent No.:** **US 10,898,324 B2**  
(45) **Date of Patent:** **Jan. 26, 2021**

(54) **TRANSCATHETER DELIVERY SYSTEM WITH WHEEL ACTUATION**

(71) Applicant: **St. Jude Medical, Cardiology Division, Inc.**, St. Paul, MN (US)

(72) Inventors: **Michael Shane Morrissey**, St. Paul, MN (US); **Bruce Edward Frohman**, Saint Louis Park, MN (US); **Michael William Metz**, Minneapolis, MN (US); **Janis Paulis Skujins**, Minneapolis, MN (US); **David John Copeland**, Minnetonka, MN (US); **Spencer Patrick Brown**, Providence, RI (US)

(73) Assignee: **St. Jude Medical, Cardiology Division, Inc.**, St. Paul, MN (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 94 days.

(21) Appl. No.: **15/976,282**

(22) Filed: **May 10, 2018**

(65) **Prior Publication Data**  
US 2018/0325669 A1 Nov. 15, 2018

**Related U.S. Application Data**

(60) Provisional application No. 62/506,251, filed on May 15, 2017.

(51) **Int. Cl.**  
*A61F 2/24* (2006.01)  
*A61F 2/95* (2013.01)

(52) **U.S. Cl.**  
CPC ..... *A61F 2/2436* (2013.01); *A61F 2/2418* (2013.01); *A61F 2/95* (2013.01); *A61F 2/9517* (2020.05)

(58) **Field of Classification Search**  
CPC .. A61F 2/2427; A61F 2/95; A61F 2002/2436; A61F 2002/9517

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,657,744 A 4/1972 Ersek  
4,275,469 A 6/1981 Gabbay  
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2011202175 B1 7/2011  
DE 19857887 A1 7/2000  
(Continued)

OTHER PUBLICATIONS

International Search Report and Written Opinion for PCT/US2018/031973, dated Oct. 19, 2018.

(Continued)


*Primary Examiner* — Todd J Scherbel

(74) *Attorney, Agent, or Firm* — Lerner, David, Littenberg, Krumholz & Mentlik, LLP

(57) **ABSTRACT**

A delivery device **1010** for a collapsible prosthetic heart valve **200**, the delivery device including an inner shaft **1026**, a distal sheath **1024** disposed about a portion of the inner shaft and forming a compartment **1023** with the inner shaft, the compartment being adapted to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle **1020** including a frame **1030** having a longitudinal axis, a proximal end and a distal end, the handle further including a deployment actuator **1021** and a hub **1100**, each of the deployment actuator and the hub being independently capable of opening and closing the compartment, the hub further including a hub actuator **1600** coupled to the inner shaft.

**15 Claims, 16 Drawing Sheets**

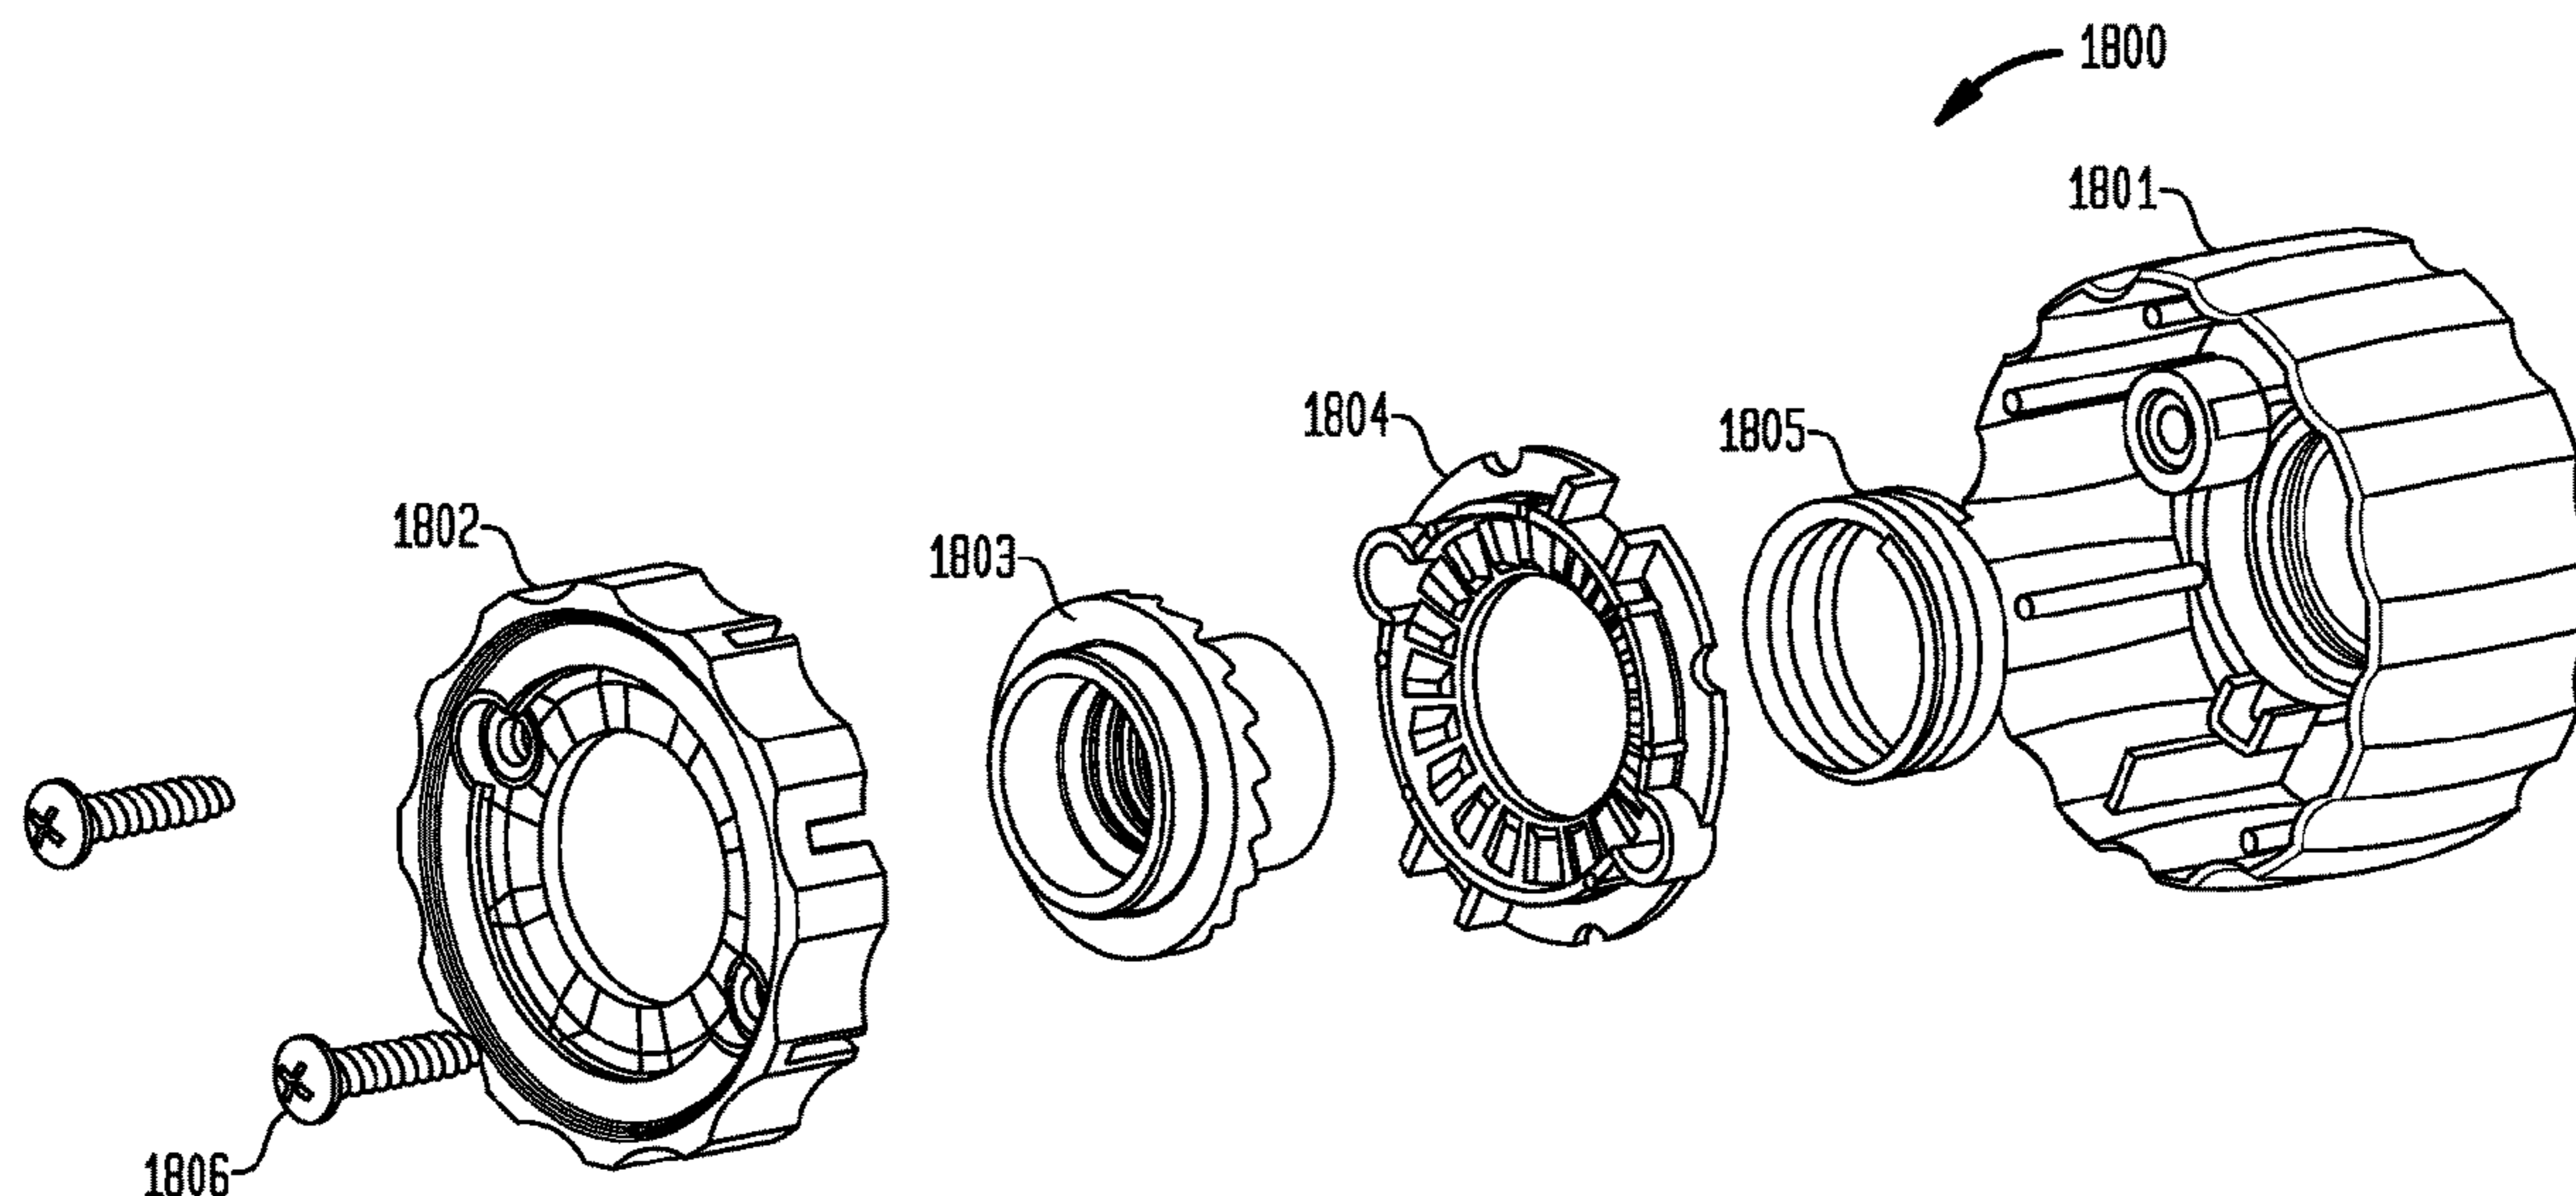



(56)

References Cited

FOREIGN PATENT DOCUMENTS

U.S. PATENT DOCUMENTS

2008/0004688 A1 1/2008 Spenser et al.  
 2008/0009940 A1 1/2008 Cribier  
 2008/0021552 A1 1/2008 Gabbay  
 2008/0039934 A1 2/2008 Styrac  
 2008/0071369 A1 3/2008 Tuval et al.  
 2008/0082159 A1 4/2008 Tseng et al.  
 2008/0097595 A1 4/2008 Gabbay  
 2008/0114452 A1 5/2008 Gabbay  
 2008/0125853 A1 5/2008 Bailey et al.  
 2008/0140189 A1 6/2008 Nguyen et al.  
 2008/0147179 A1 6/2008 Cai et al.  
 2008/0147182 A1 6/2008 Righini et al.  
 2008/0147183 A1 6/2008 Styrac  
 2008/0154355 A1 6/2008 Benichou et al.  
 2008/0154356 A1 6/2008 Obermiller et al.  
 2008/0228264 A1 9/2008 Li et al.  
 2008/0243245 A1 10/2008 Thambar et al.  
 2008/0255662 A1 10/2008 Stacchino et al.  
 2008/0262602 A1 10/2008 Wilk et al.  
 2008/0269878 A1 10/2008 Iobbi  
 2008/0269879 A1 10/2008 Sathe et al.  
 2009/0024137 A1 1/2009 Chuter et al.  
 2009/0054975 A1 2/2009 del Nido et al.  
 2009/0105798 A1 4/2009 Koch  
 2009/0112309 A1 4/2009 Jaramillo et al.  
 2009/0118826 A1 5/2009 Khaghani  
 2009/0138079 A1 5/2009 Tuval et al.  
 2009/0287299 A1 11/2009 Tabor et al.  
 2010/0004740 A1 1/2010 Seguin et al.  
 2010/0036484 A1 2/2010 Hariton et al.  
 2010/0049306 A1 2/2010 House et al.  
 2010/0049313 A1 2/2010 Alon et al.  
 2010/0082094 A1 4/2010 Quadri et al.  
 2010/0087907 A1 4/2010 Lattouf  
 2010/0114305 A1 5/2010 Kang et al.  
 2010/0121434 A1 5/2010 Paul et al.  
 2010/0131055 A1 5/2010 Case et al.  
 2010/0168778 A1 7/2010 Braido  
 2010/0168839 A1 7/2010 Braido et al.  
 2010/0174290 A1 7/2010 Wuebbeling et al.  
 2010/0185277 A1 7/2010 Braido et al.  
 2010/0191326 A1 7/2010 Alkhatib  
 2010/0204781 A1 8/2010 Alkhatib  
 2010/0204785 A1 8/2010 Alkhatib  
 2010/0217382 A1 8/2010 Chau et al.  
 2010/0249911 A1 9/2010 Alkhatib  
 2010/0249923 A1 9/2010 Alkhatib et al.  
 2010/0286768 A1 11/2010 Alkhatib  
 2010/0298931 A1 11/2010 Quadri et al.  
 2011/0029072 A1 2/2011 Gabbay  
 2011/0208298 A1 8/2011 Tuval et al.  
 2011/0224678 A1 9/2011 Gabbay  
 2011/0282425 A1 11/2011 Dwork  
 2011/0288626 A1 11/2011 Straubinger et al.  
 2011/0295216 A1 12/2011 Miller  
 2012/0022635 A1 1/2012 Yamashita  
 2012/0053574 A1 3/2012 Murray, III et al.  
 2012/0078352 A1 3/2012 Wang et al.  
 2012/0197391 A1 8/2012 Alkhatib et al.  
 2012/0310332 A1 12/2012 Murray et al.  
 2013/0030520 A1 1/2013 Lee et al.  
 2013/0131774 A1\* 5/2013 Nabulsi ..... A61F 2/95  
 623/1.11  
 2013/0138118 A1 5/2013 Doyle  
 2013/0231735 A1 9/2013 Deem et al.  
 2013/0297011 A1 11/2013 Morris et al.  
 2013/0304179 A1 11/2013 Bialas et al.  
 2014/0067050 A1 3/2014 Costello et al.  
 2014/0135909 A1 5/2014 Carr et al.  
 2014/0343670 A1 11/2014 Bakis et al.  
 2015/0305867 A1 10/2015 Liu et al.  
 2017/0056169 A1 3/2017 Johnson et al.

DE 20000659 U1 5/2001  
 DE 10121210 A1 11/2002  
 DE 202008009610 U1 12/2008  
 EP 0850607 A1 7/1998  
 EP 1000590 A1 5/2000  
 EP 1129744 A1 9/2001  
 EP 1157673 A2 11/2001  
 EP 1360942 A1 11/2003  
 EP 1584306 A1 10/2005  
 EP 1598031 A2 11/2005  
 FR 2847800 B1 10/2005  
 JP 2001504717 A 4/2001  
 JP 2003334254 A 11/2003  
 JP 2004130074 4/2004  
 JP 2010504820 A 2/2010  
 JP 2010526609 A 8/2010  
 JP 2010531193 9/2010  
 JP 2012500665 A 1/2012  
 WO 9117720 A1 11/1991  
 WO 9716133 A1 5/1997  
 WO 9832412 A2 7/1998  
 WO 9913801 A1 3/1999  
 WO 0018330 A1 4/2000  
 WO 0069368 A2 11/2000  
 WO 0128459 A1 4/2001  
 WO 0149213 A2 7/2001  
 WO 0154625 A1 8/2001  
 WO 0156500 A2 8/2001  
 WO 0176510 A2 10/2001  
 WO 0236048 A1 5/2002  
 WO 0247575 A2 6/2002  
 WO 03047468 A1 6/2003  
 WO 06073626 A2 7/2006  
 WO 07071436 A2 6/2007  
 WO 2008042266 A2 4/2008  
 WO 08070797 A2 6/2008  
 WO 2008138584 A1 11/2008  
 WO 2009001309 12/2008  
 WO 2009011866 A1 1/2009  
 WO 2009029199 A1 3/2009  
 WO 2009042196 A2 4/2009  
 WO 2009091509 A1 7/2009  
 WO 2010008548 A2 1/2010  
 WO 2010008549 A1 1/2010  
 WO 2010051025 A1 5/2010  
 WO 2010087975 A1 8/2010  
 WO 2010096176 A1 8/2010  
 WO 2010098857 A1 9/2010  
 WO 2011137531 A9 11/2011  
 WO 2012026965 A2 3/2012  
 WO 2012036741 A2 3/2012  
 WO 2016059084 A2 4/2016

OTHER PUBLICATIONS

Alkhatib, U.S. Appl. No. 13/216,124, filed Aug. 23, 2011, titled "Leaflet Suturing to Commissure Points for Prosthetic Heart Valve". Australian Examination Report for Application No. 2011293898 dated Jul. 26, 2013.  
 Extended European Search Report for Application No. 16196712 dated May 9, 2017.  
 International Search Report and Written Opinion for Application No. PCT/US2011/001450 dated Mar. 5, 2012.  
 International Search Report and Written Opinion for Application No. PCT/US2011/001615 dated Jul. 11, 2012.  
 International Search Report and Written Opinion for Application No. PCT/US2013/039407 dated Feb. 10, 2014.  
 International Search Report and Written Opinion for Application No. PCT/US2014/064253 dated Feb. 3, 2015.  
 International Search Report Application No. PCT/US2011/048963, dated Dec. 15, 2011.  
 International Search Report Application No. PCT/US2011/048967, dated Dec. 15, 2011.  
 International Search Report Application No. PCT/US2011/048989, dated Dec. 15, 2011.

(56)


**References Cited**

OTHER PUBLICATIONS


International Search Report for Application No. PCT/US2011/001450 dated Mar. 5, 2012.  
International Search Report for Application No. PCT/US2011/001597 dated Mar. 7, 2012.  
International Search Report for Application No. PCT/US2011/001615 dated Jul. 11, 2012.  
International Search Report for Application No. PCT/US2013/039407 dated Feb. 10, 2014.  
International Search Report for Application No. PCT/US2014/064253 dated Feb. 3, 2015.  
International Search Report from PCT/US2017/063893, dated Feb. 7, 2018, 3 pages.  
Japanese Office Action for Application No. 2013-525891 dated May 8, 2015.  
Knippel, U.S. Appl. No. 13/234,782, filed Sep. 16, 2011, titled "Staged Deployment Devices and Method for Transcatheter Heart Valve Delivery".  
Morris, U.S. Appl. No. 13/788,820, filed Mar. 7, 2013, titled "Devices and Methods for Transcatheter Heart Valve Delivery".  
Ruiz, Carlos, Overview of PRE-CE Mark Transcatheter Aortic Valve Technologies, Euro PCR, dated May 25, 2010.  
Wang, U.S. Appl. No. 13/212,442, filed Aug. 18, 2011, titled "Staged Deployment Devices and Methods for Transcatheter Heart Valve Delivery Systems".  
International Search Report for PCT/US2017/063899, dated Feb. 7, 2018, 3 pages.

\* cited by examiner

**FIG. 1**  
(PRIOR ART)

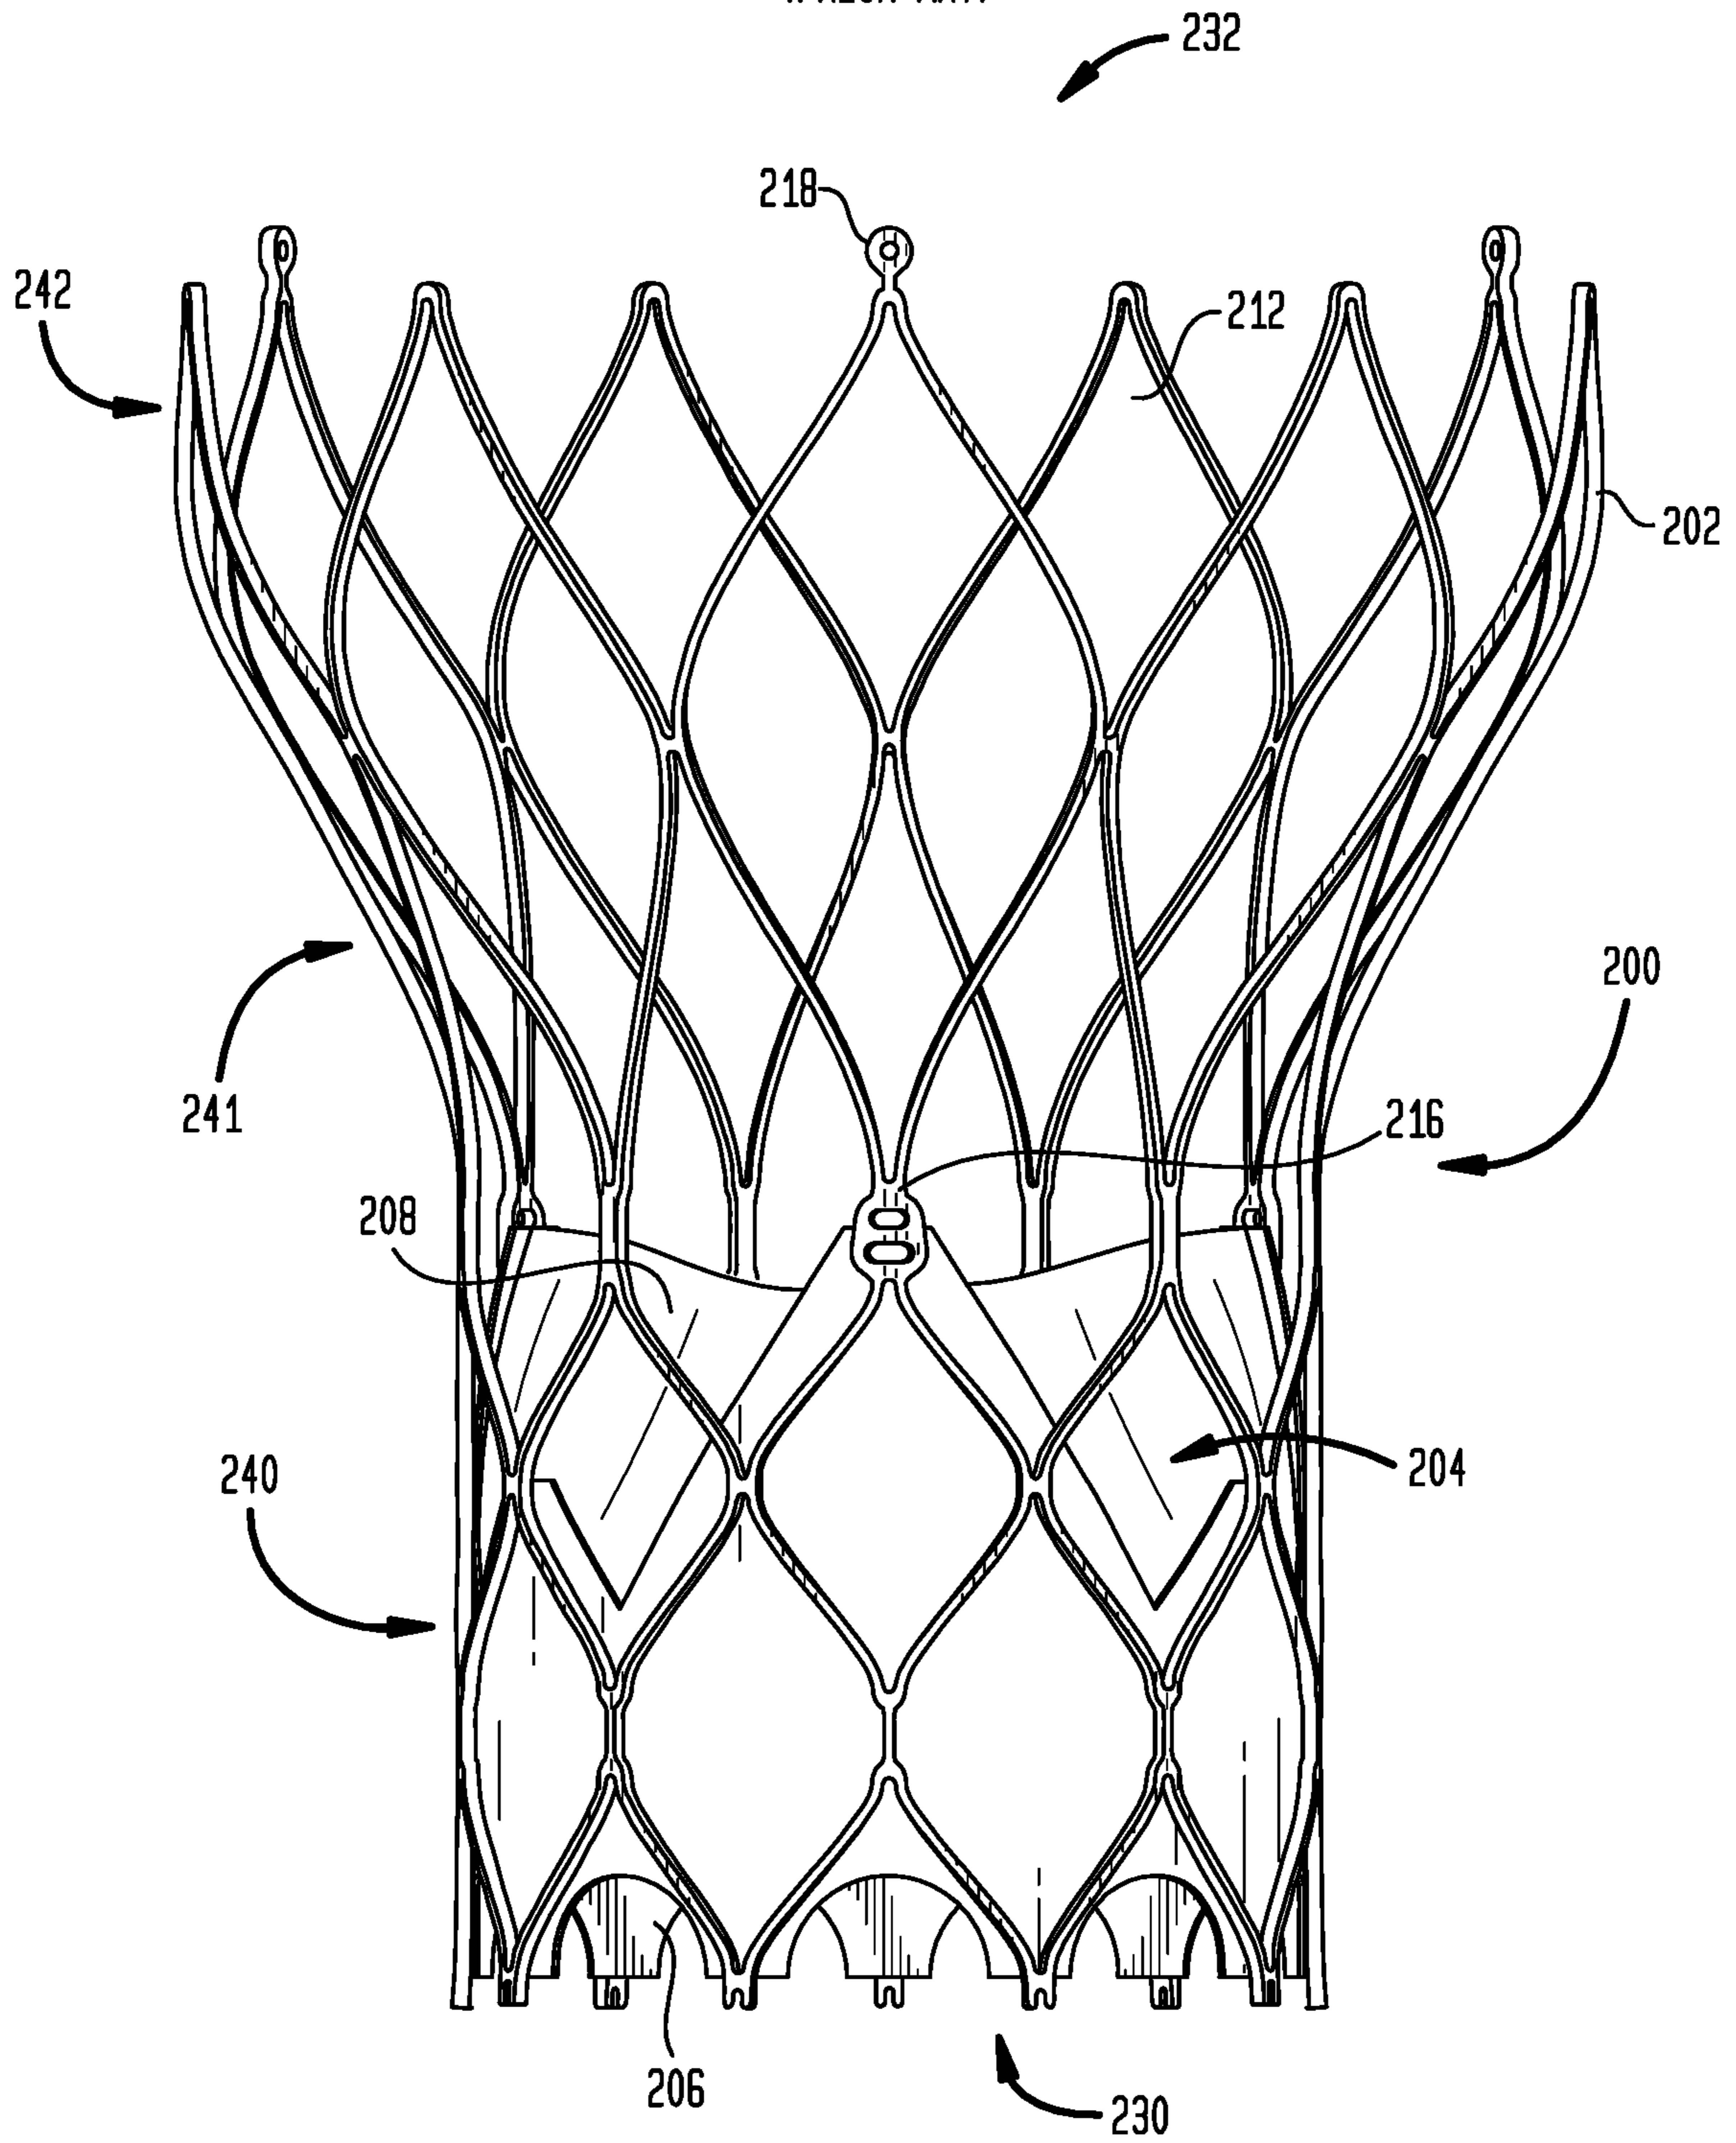

**FIG. 2A**  
(PRIOR ART)

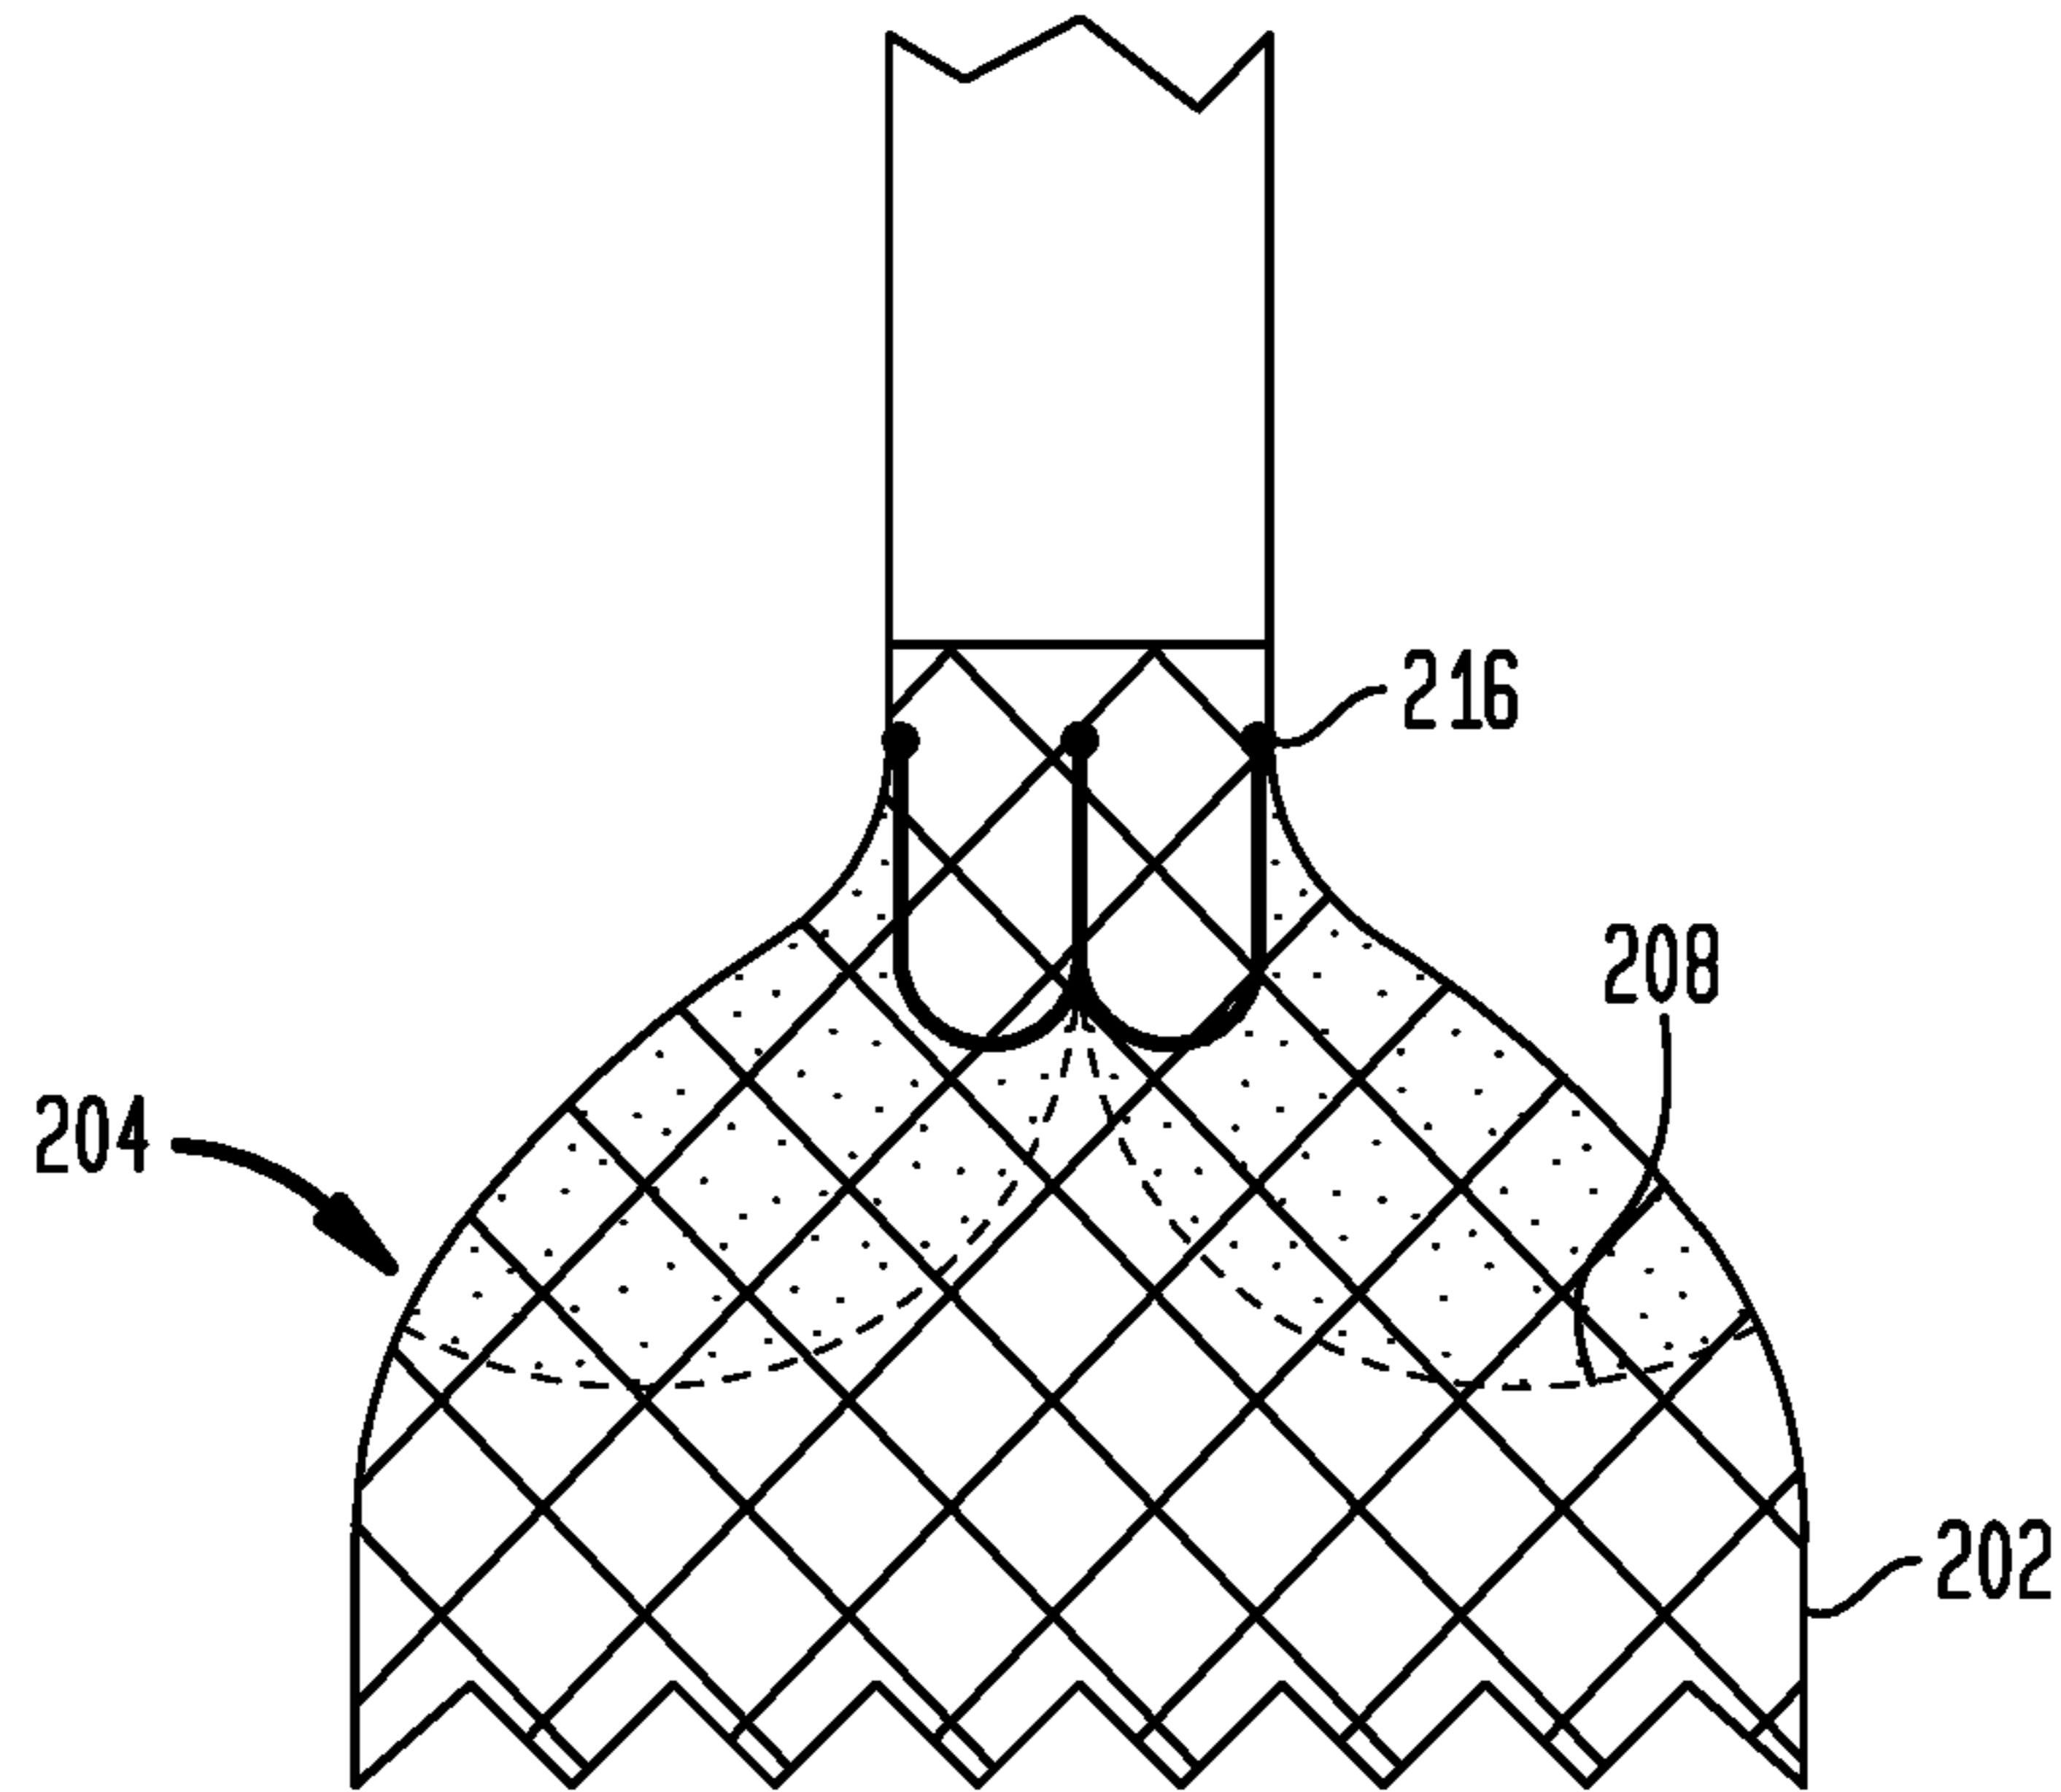

**FIG. 2B**  
(PRIOR ART)

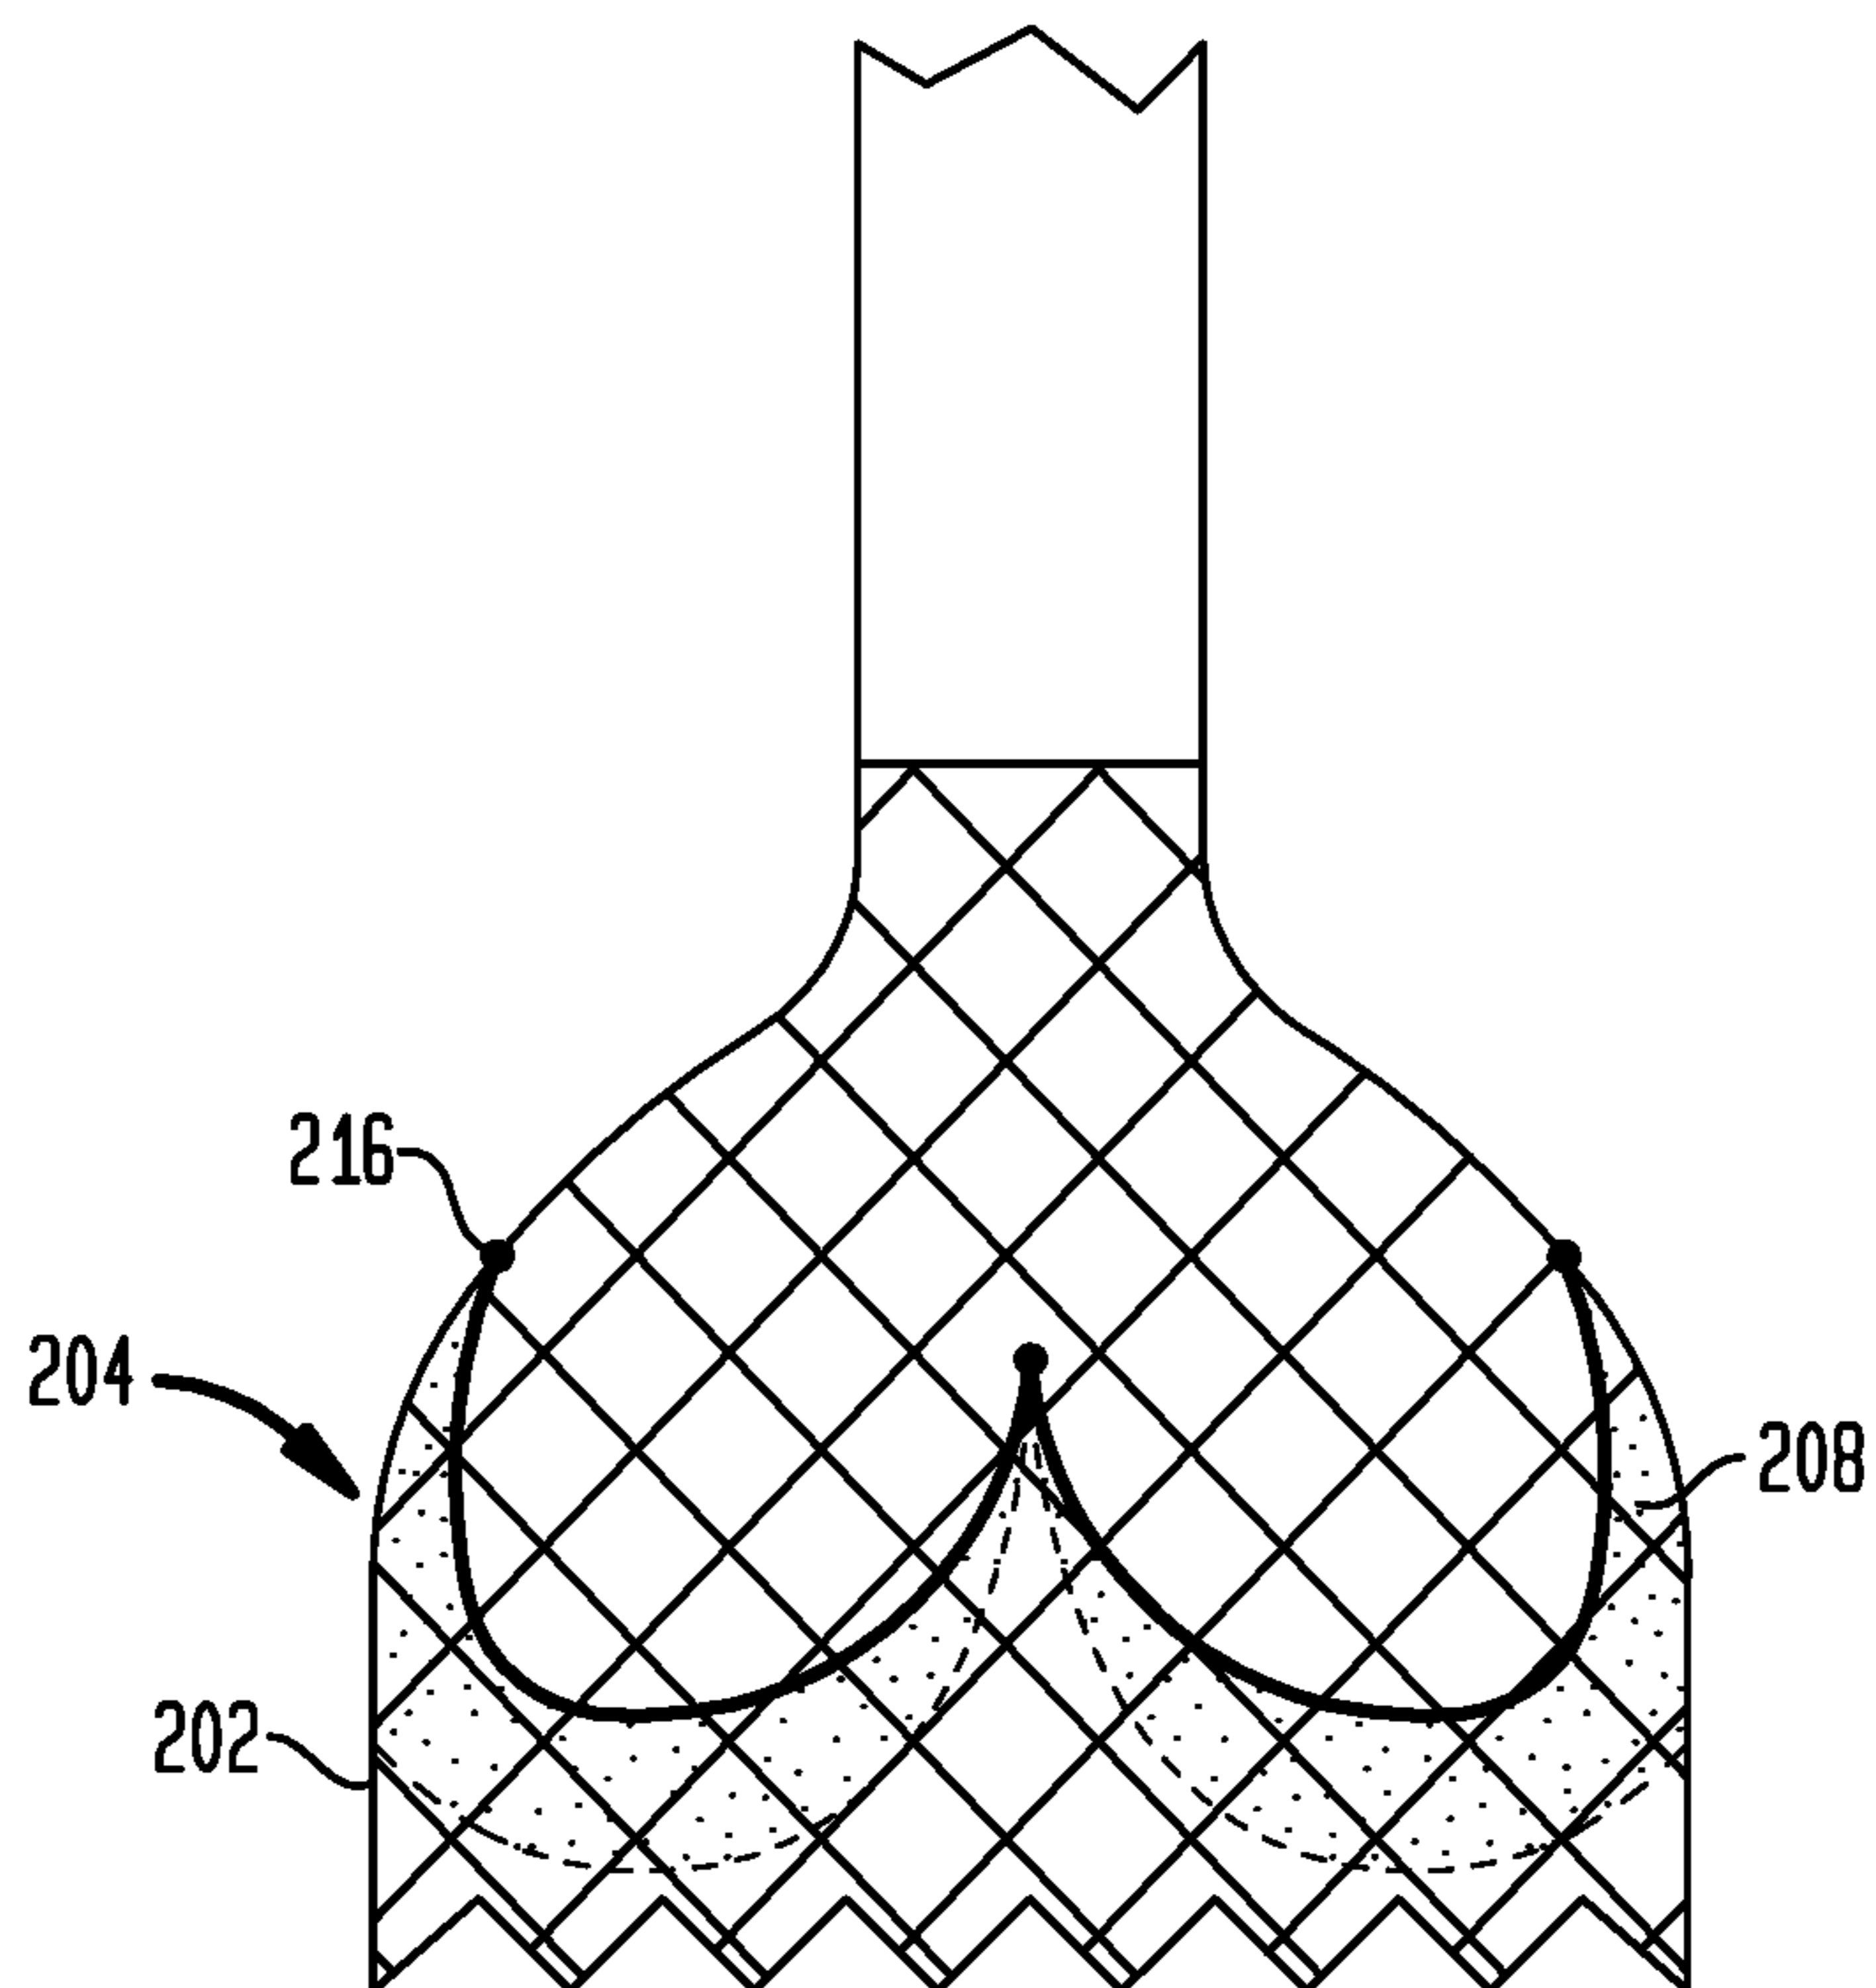


FIG. 3A

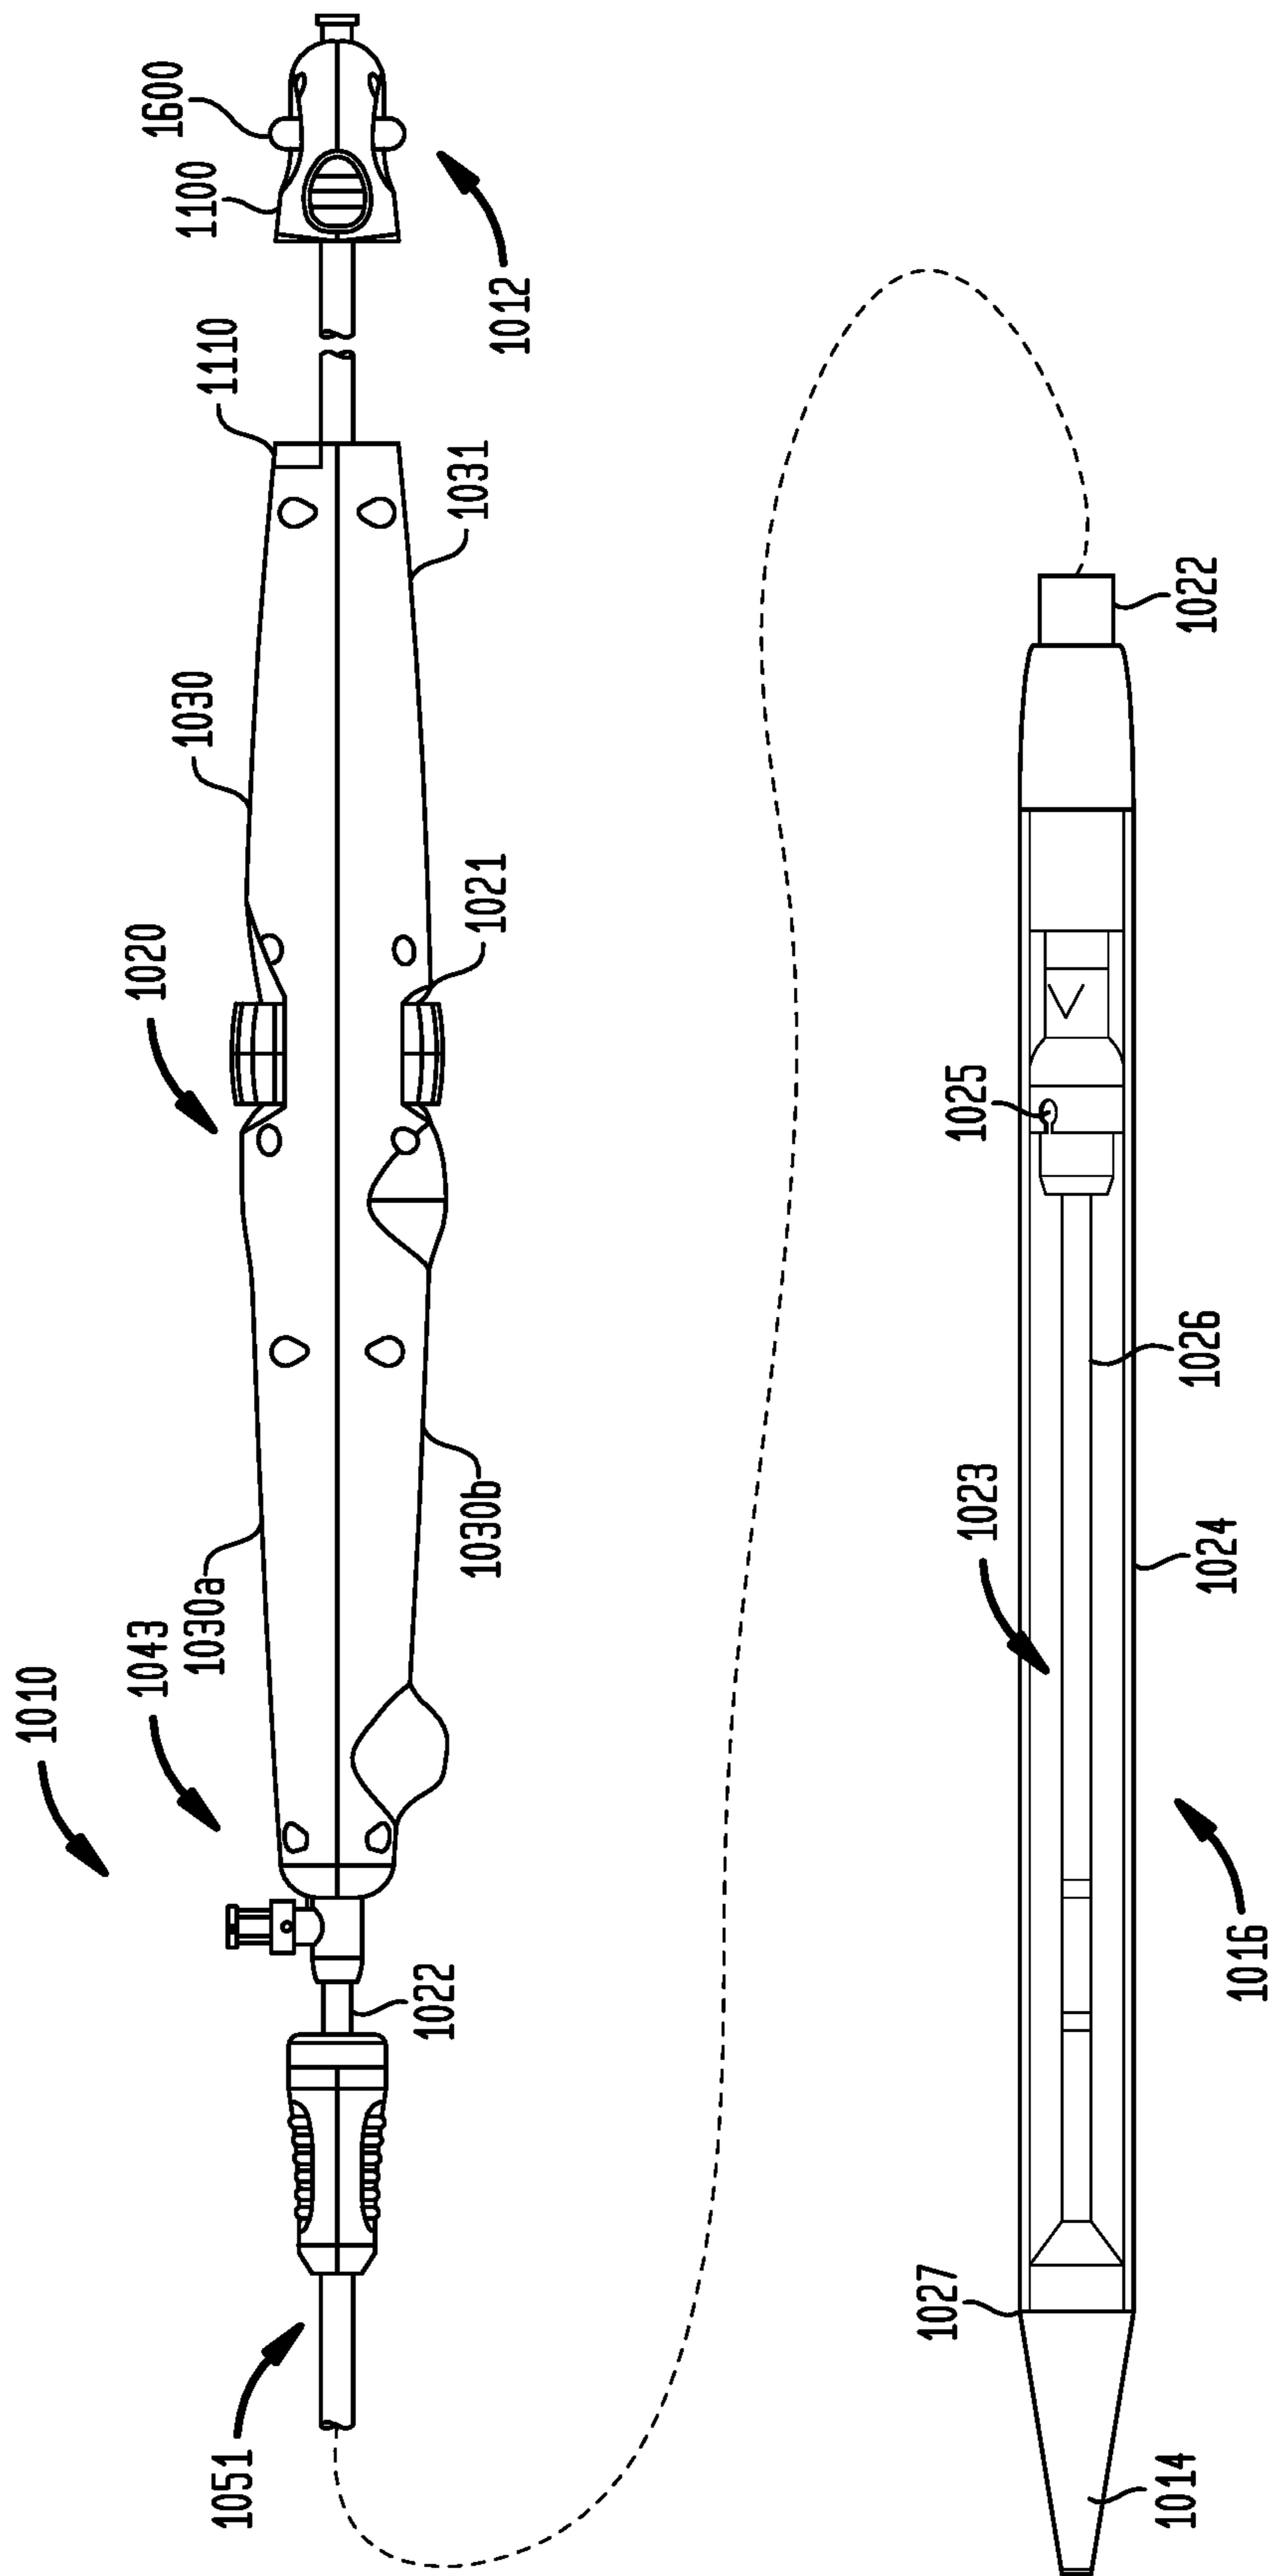


FIG. 3B

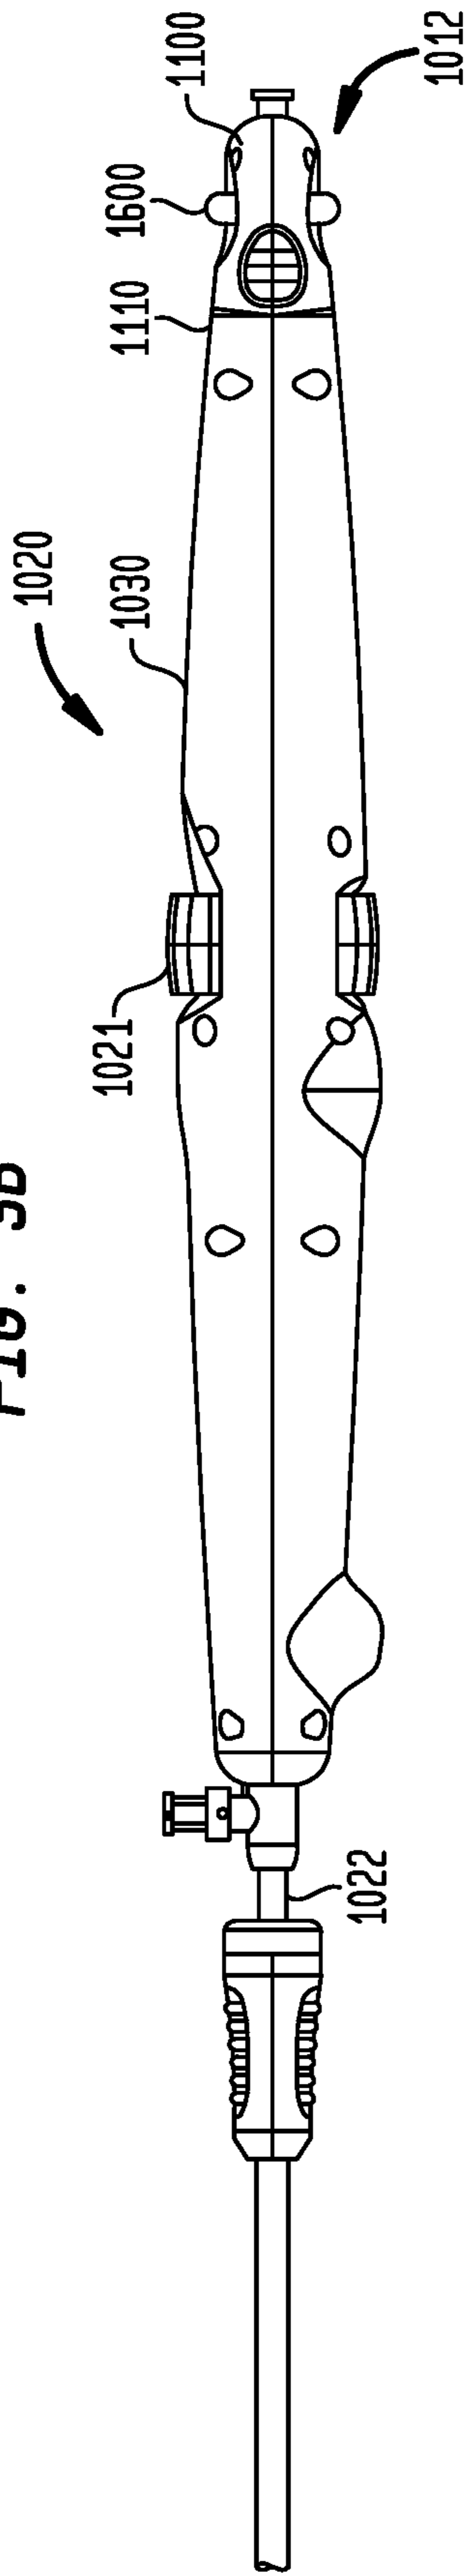


FIG. 3C

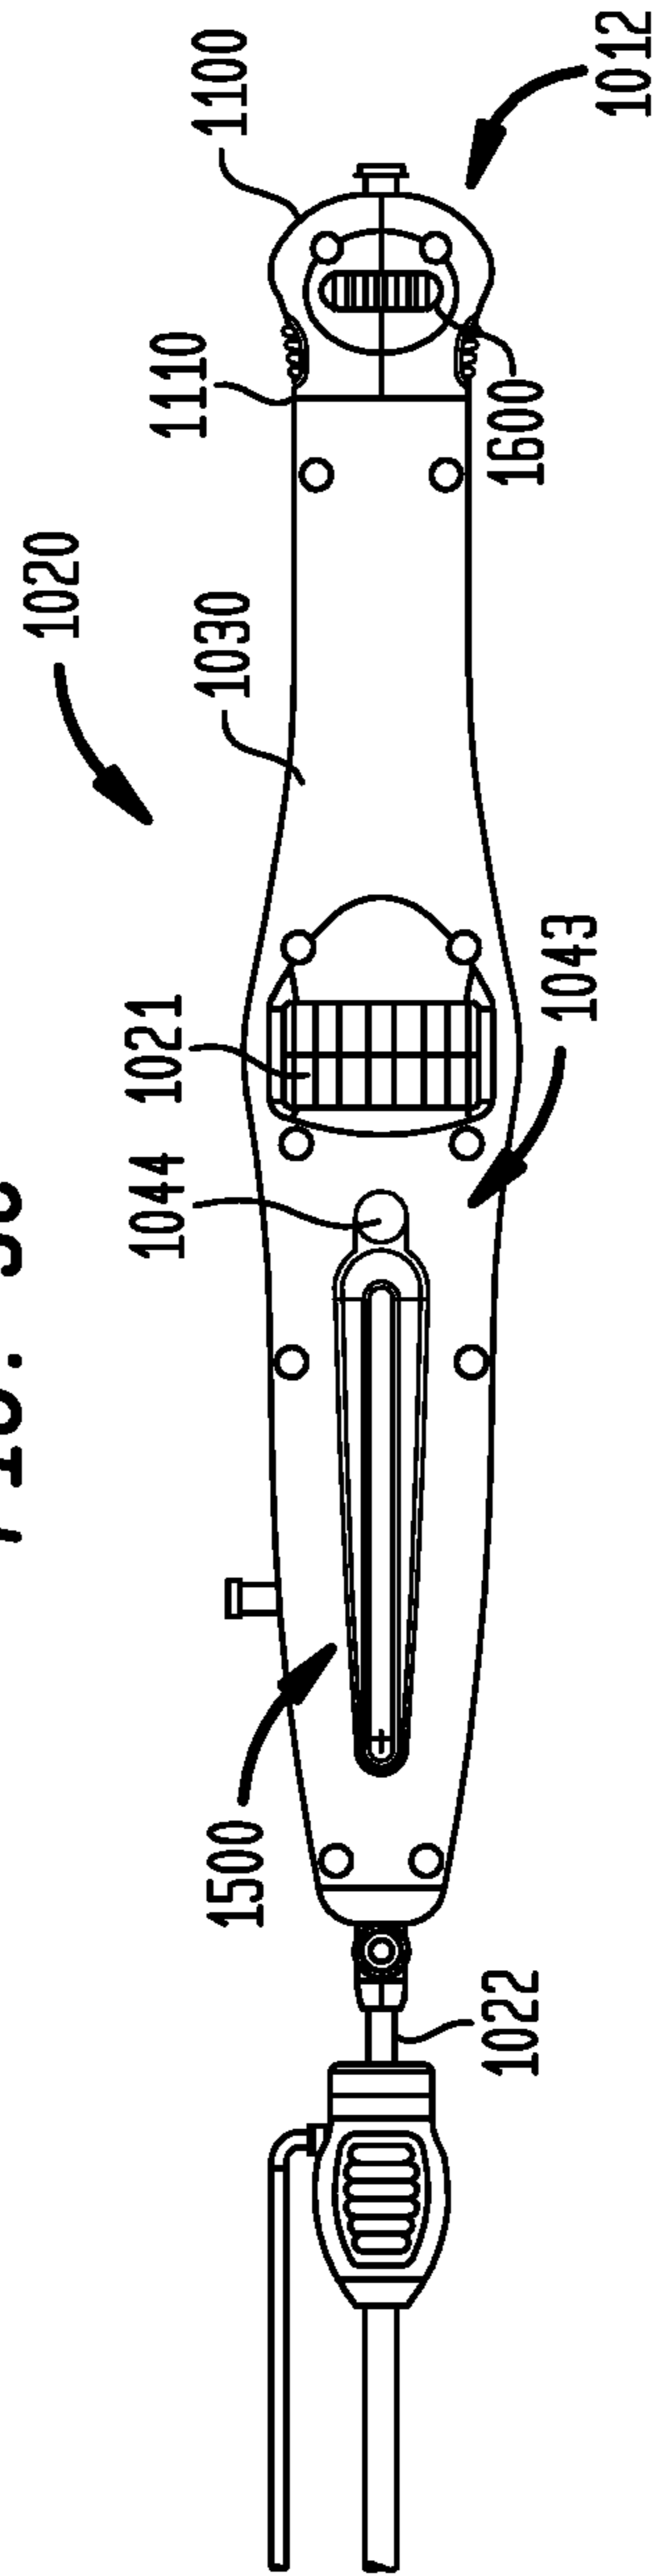


FIG. 3D

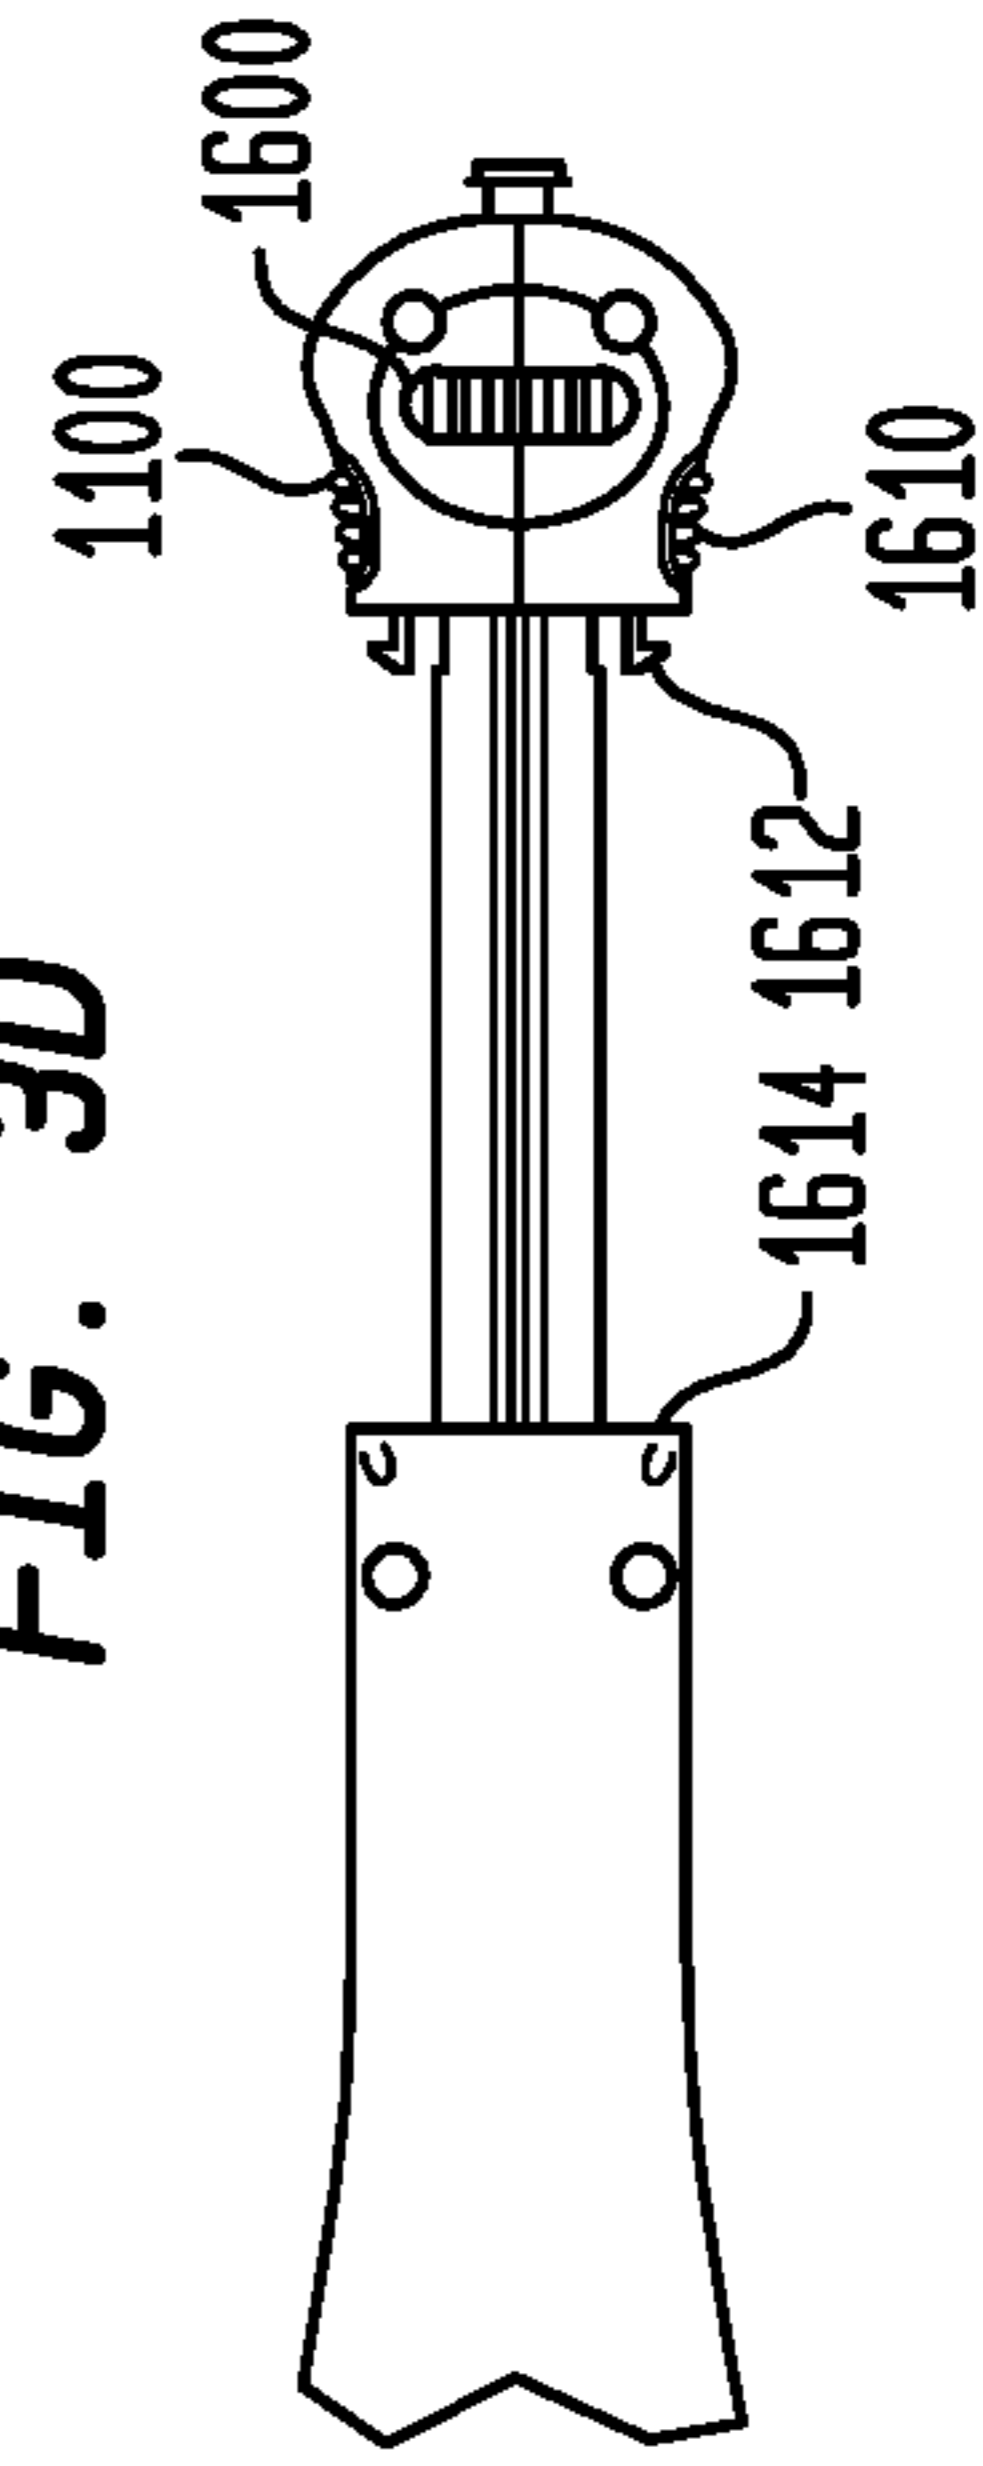




FIG. 4

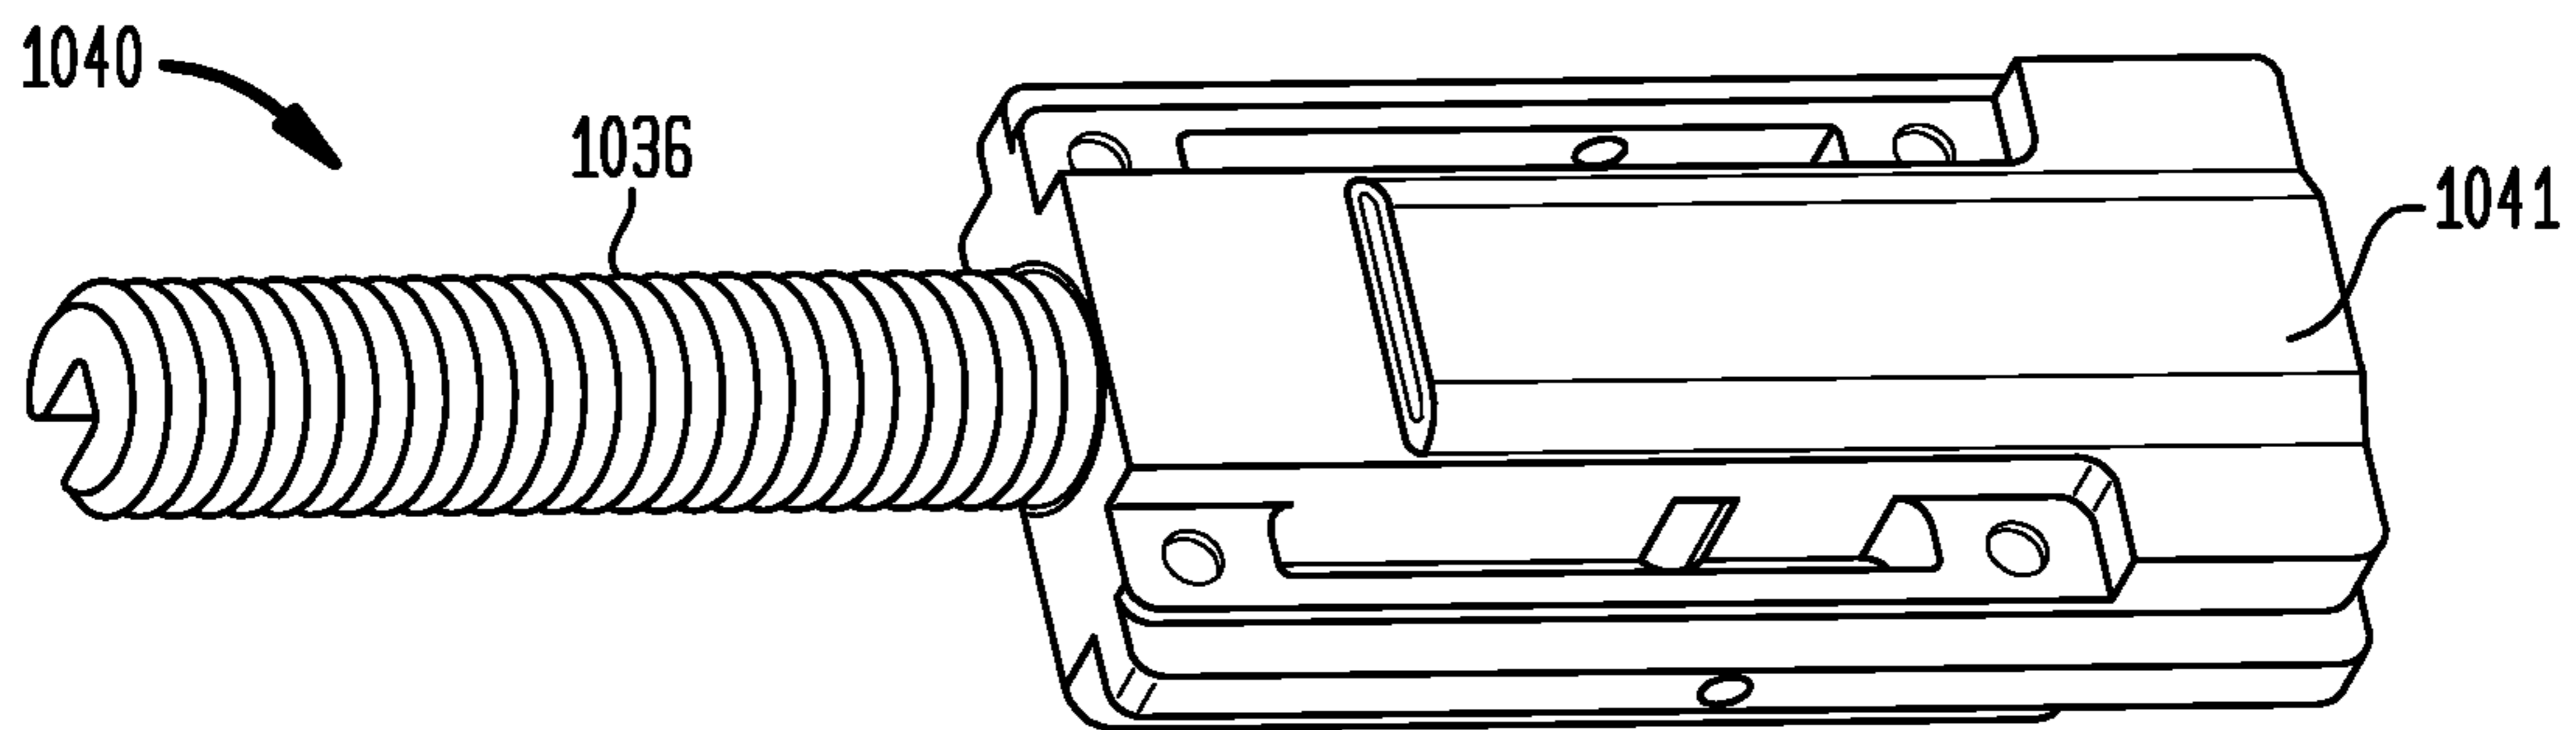


FIG. 5

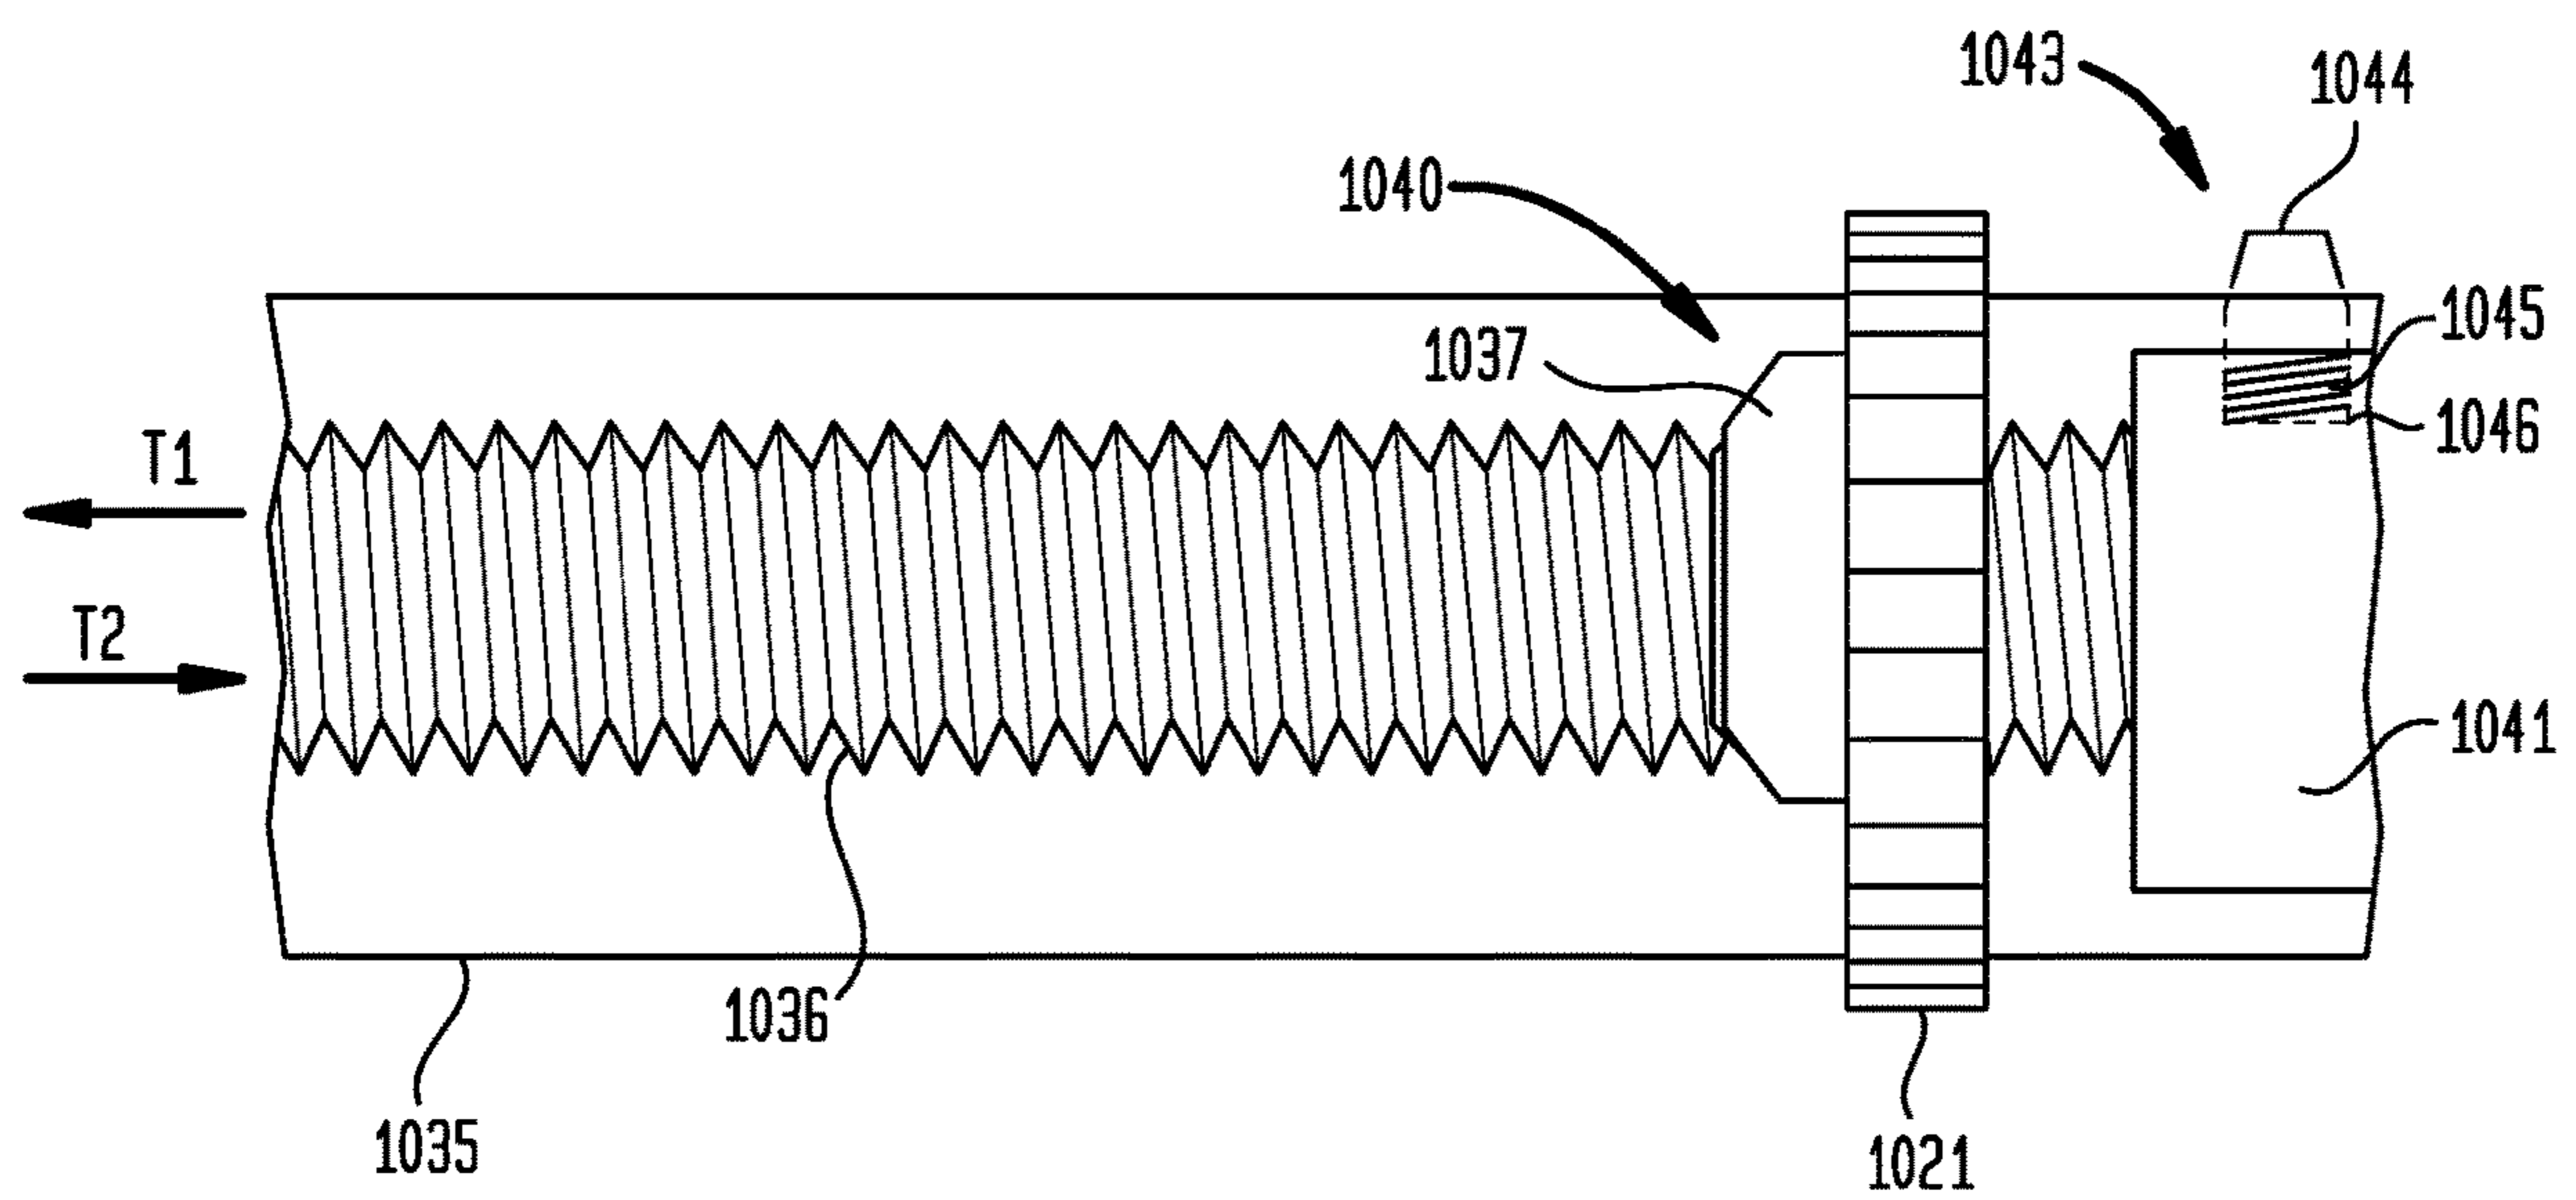


FIG. 6

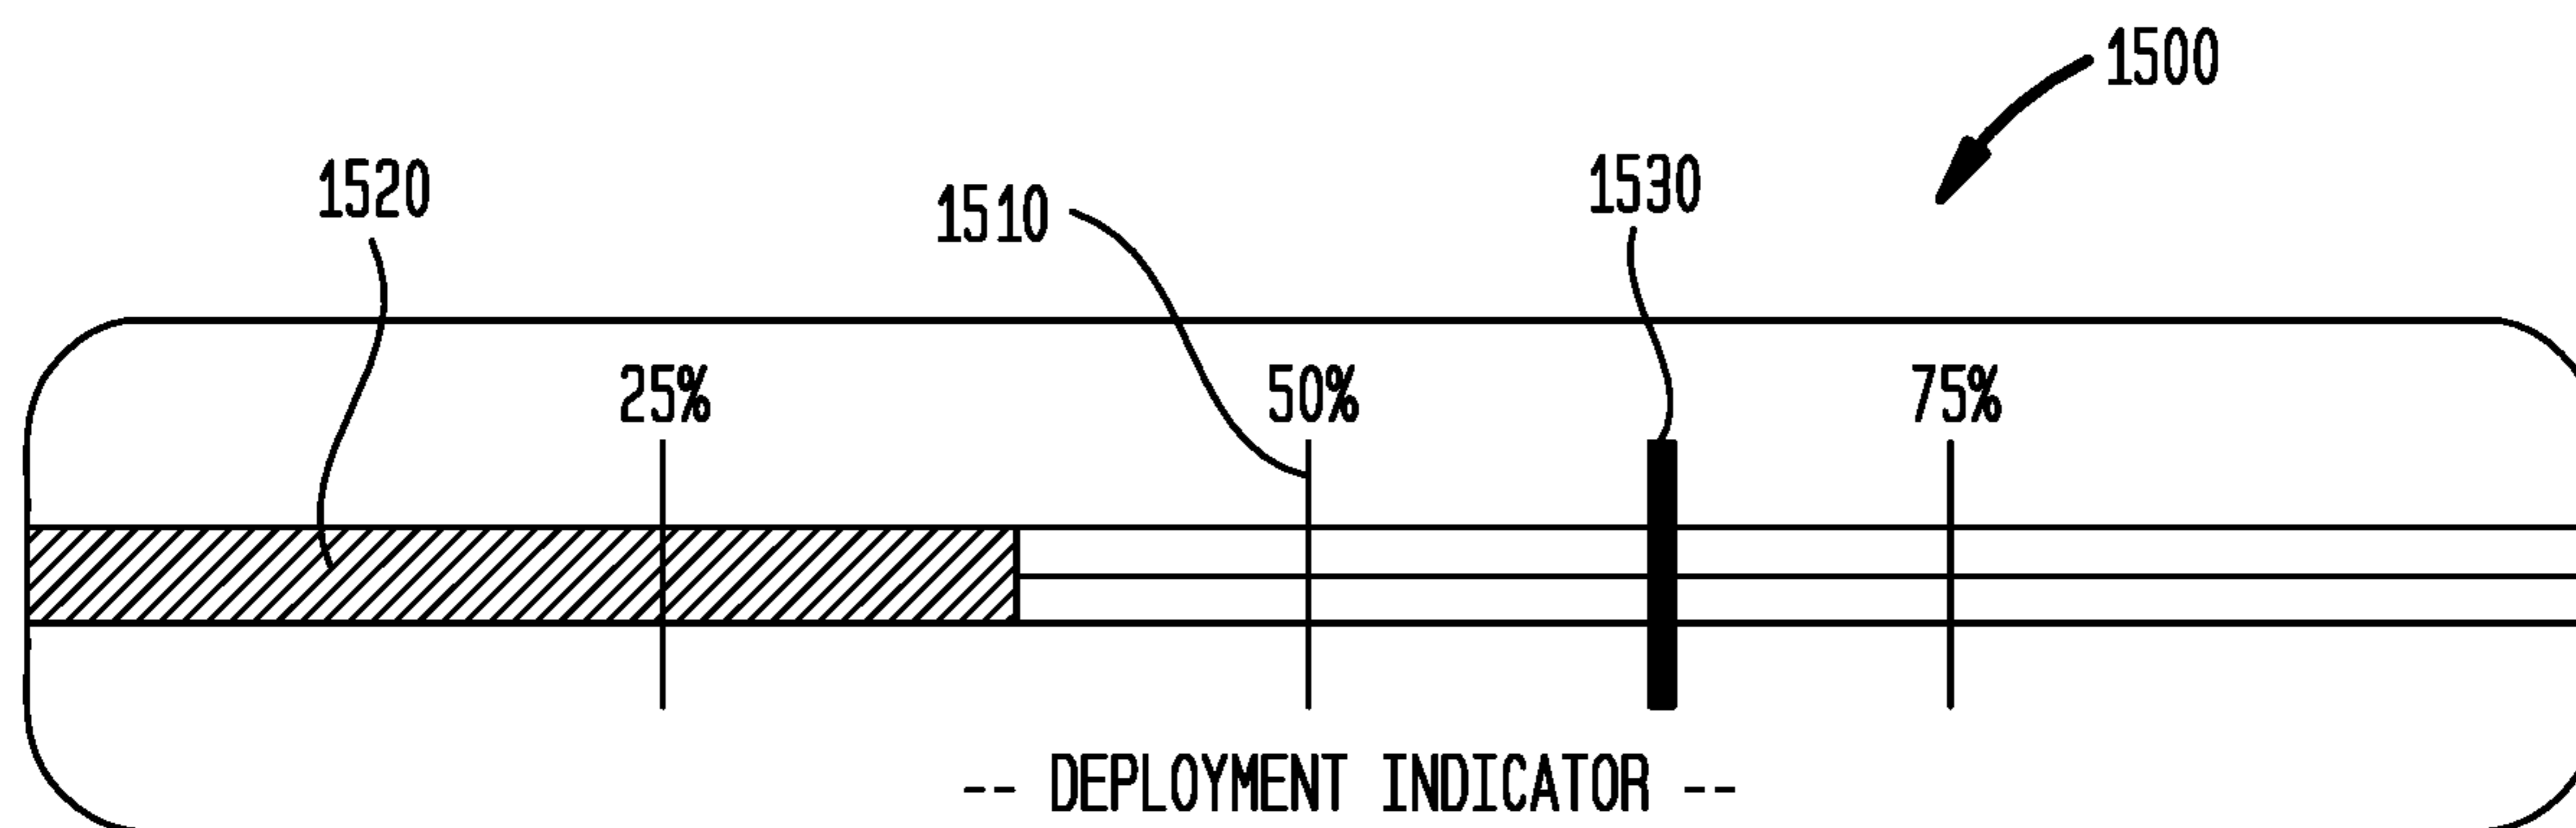


FIG. 7A

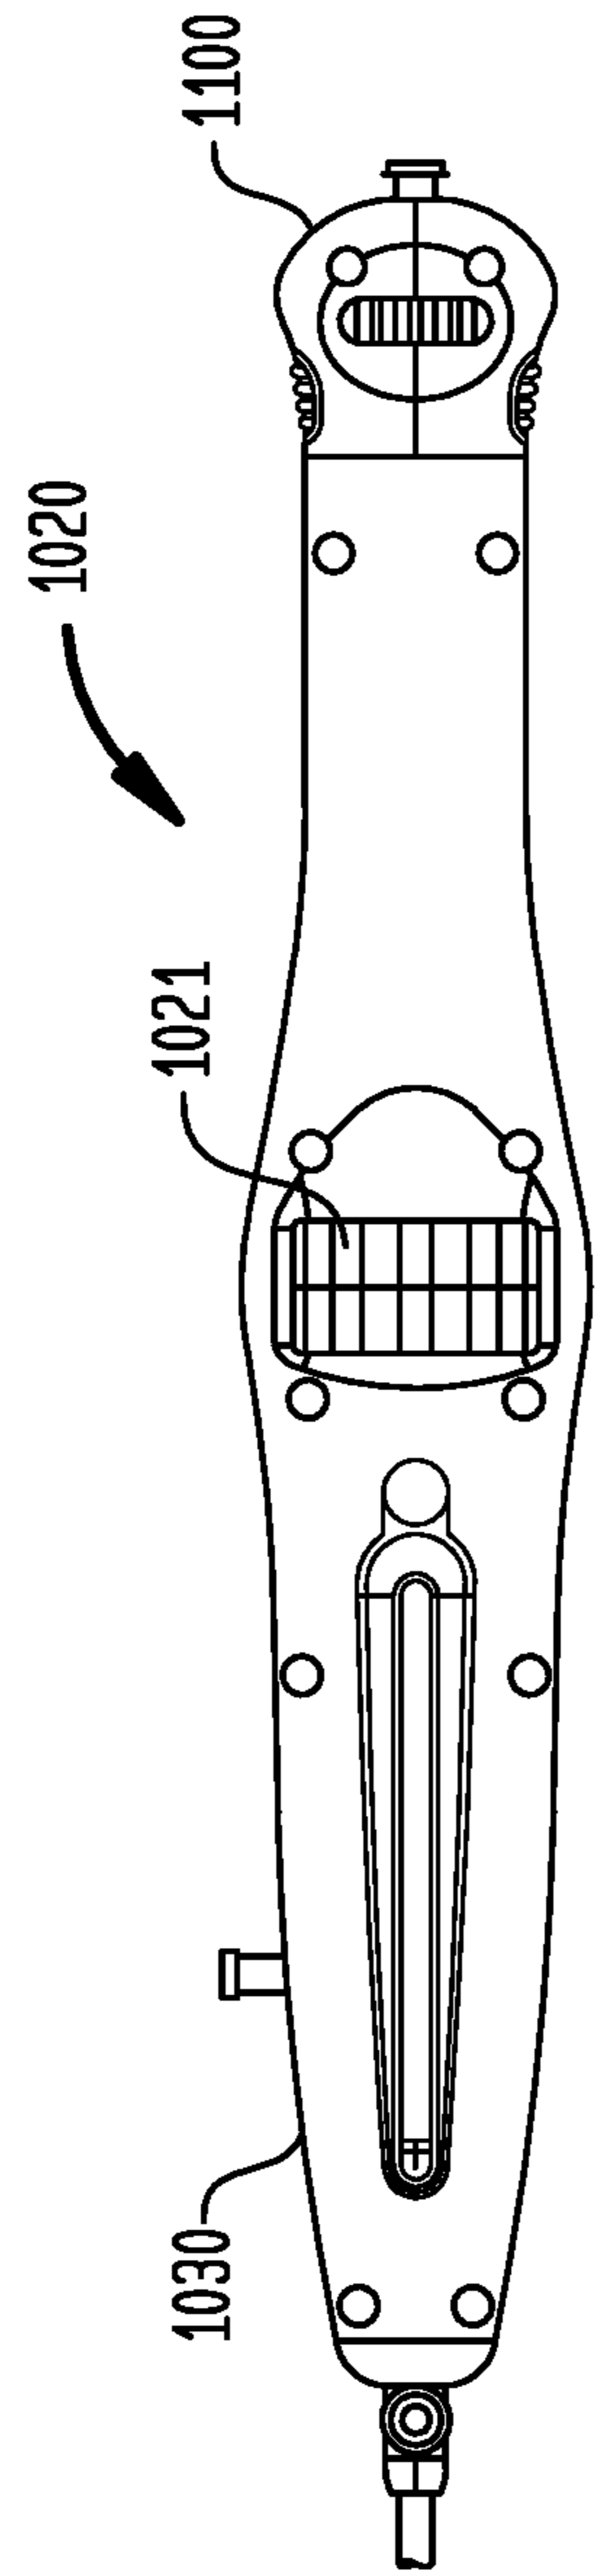


FIG. 7B

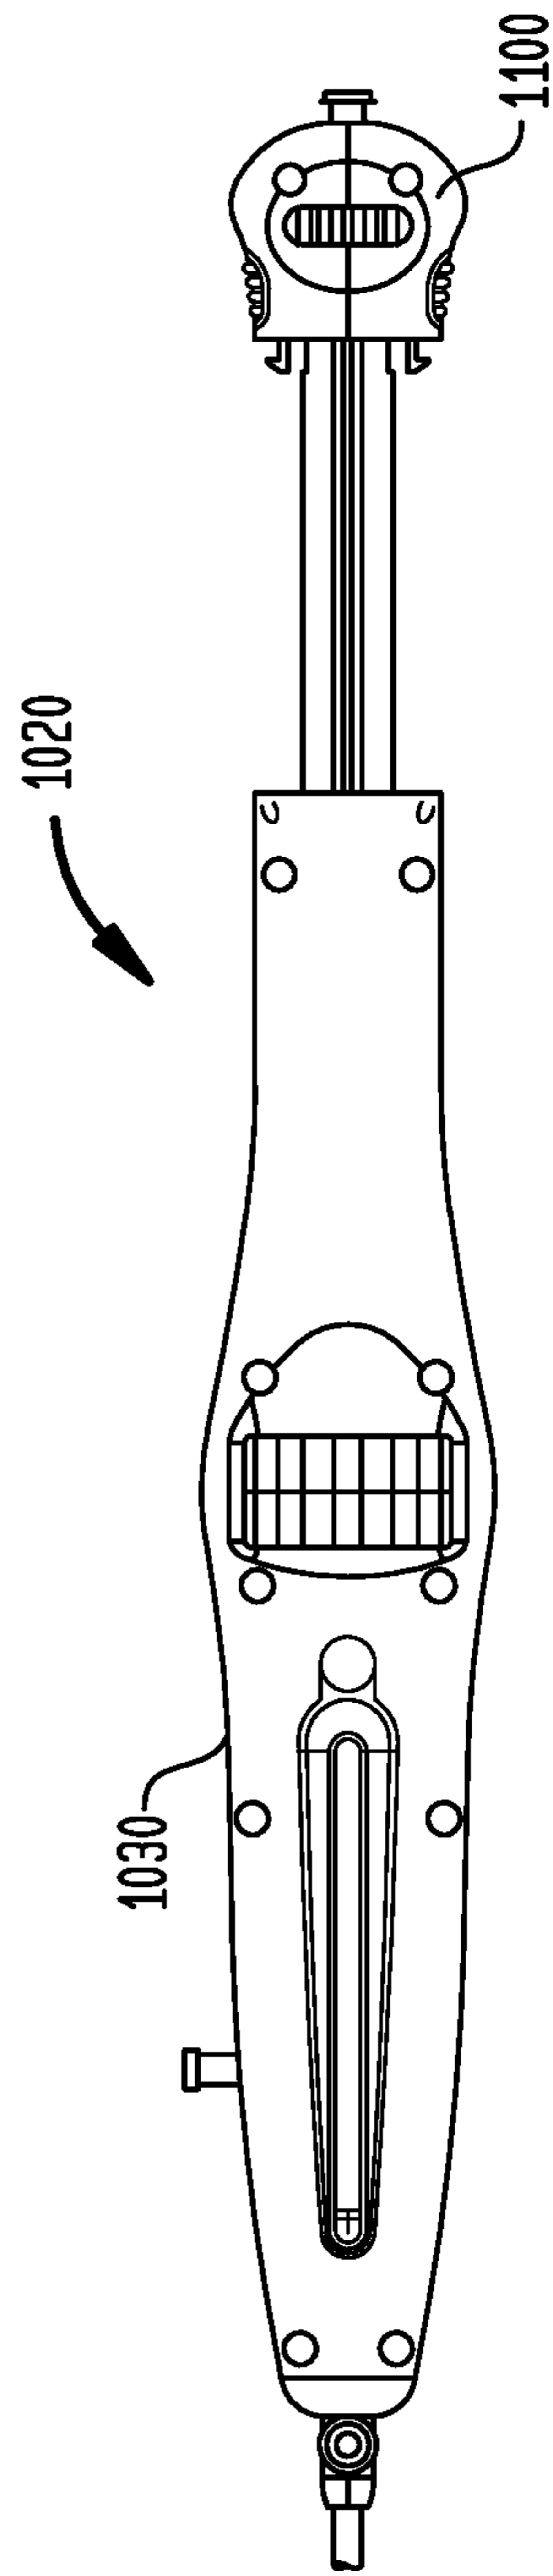


FIG. 8A

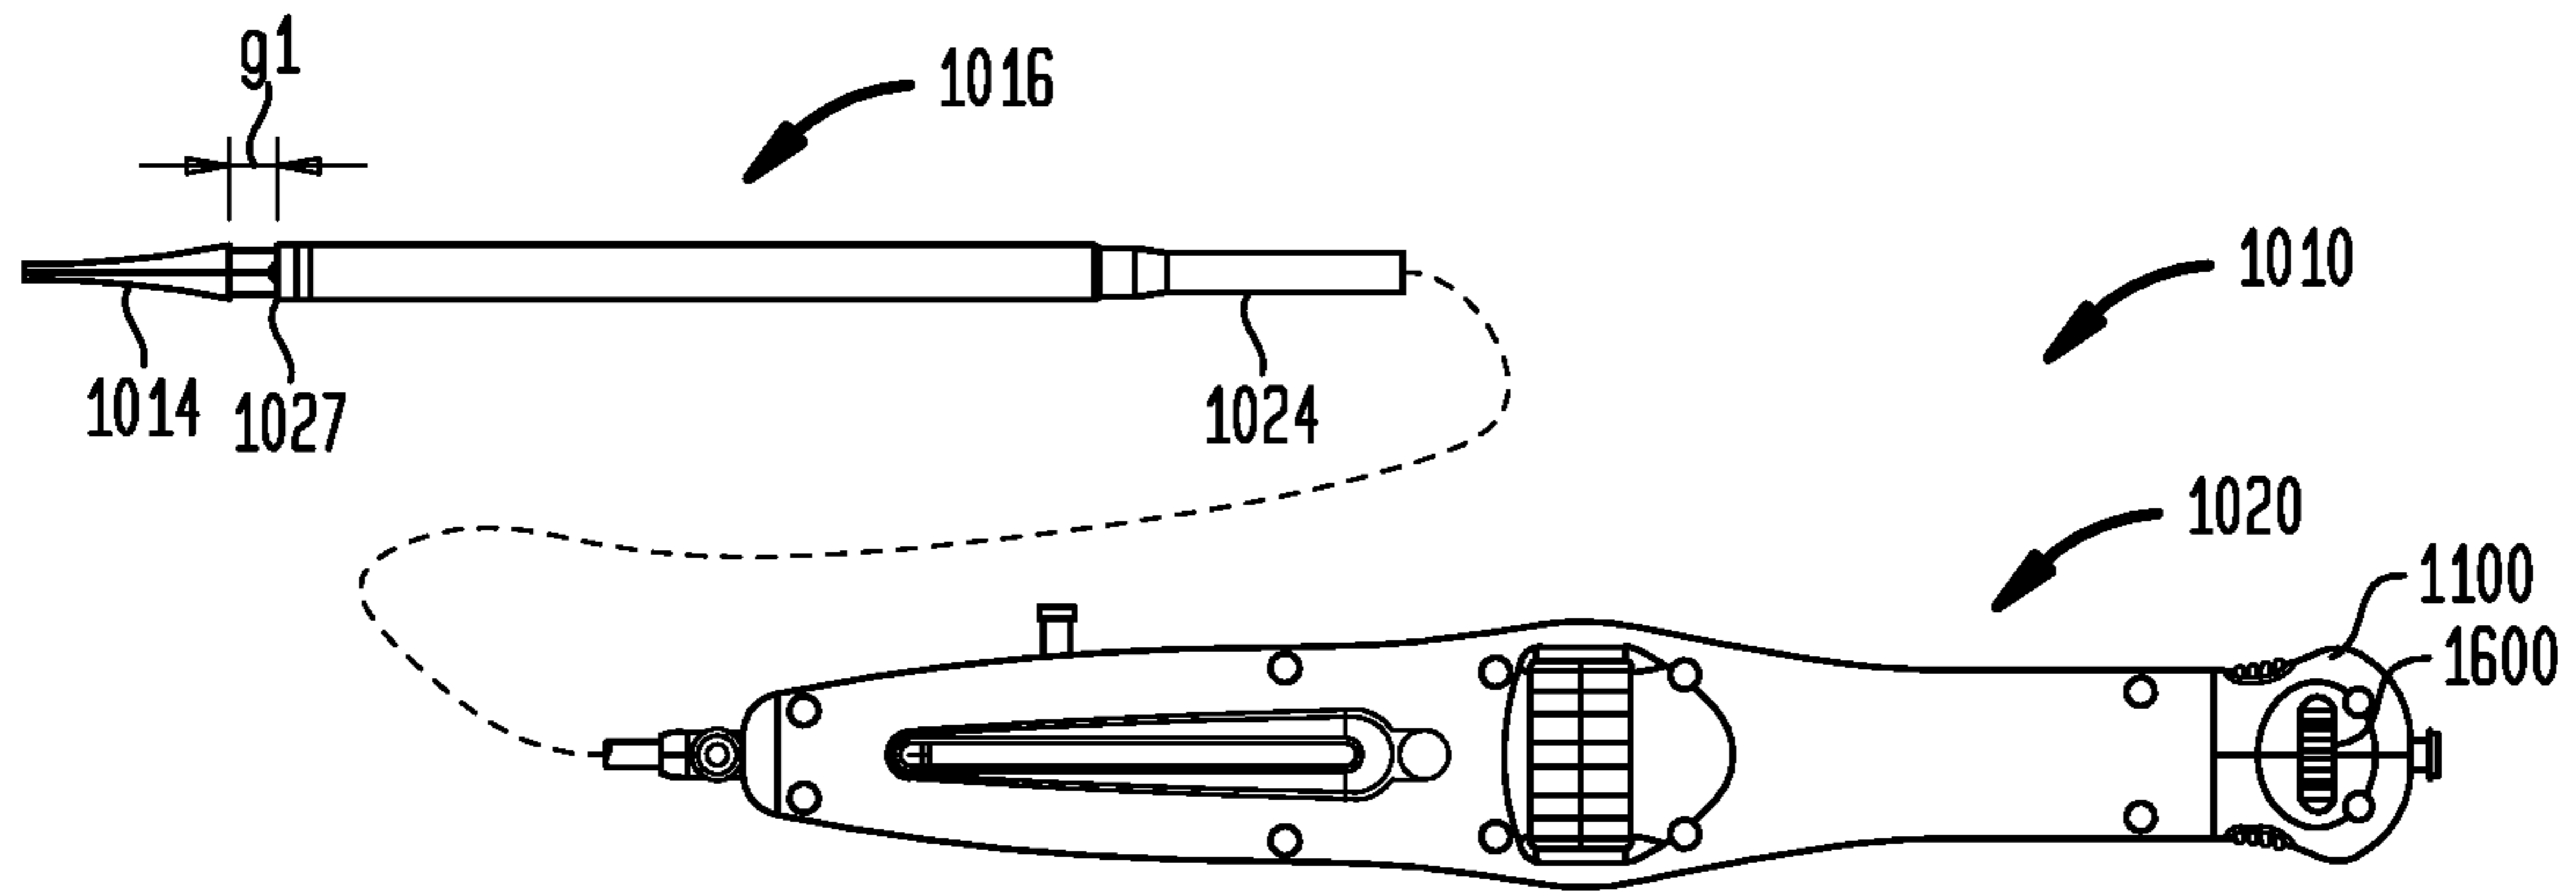


FIG. 8B

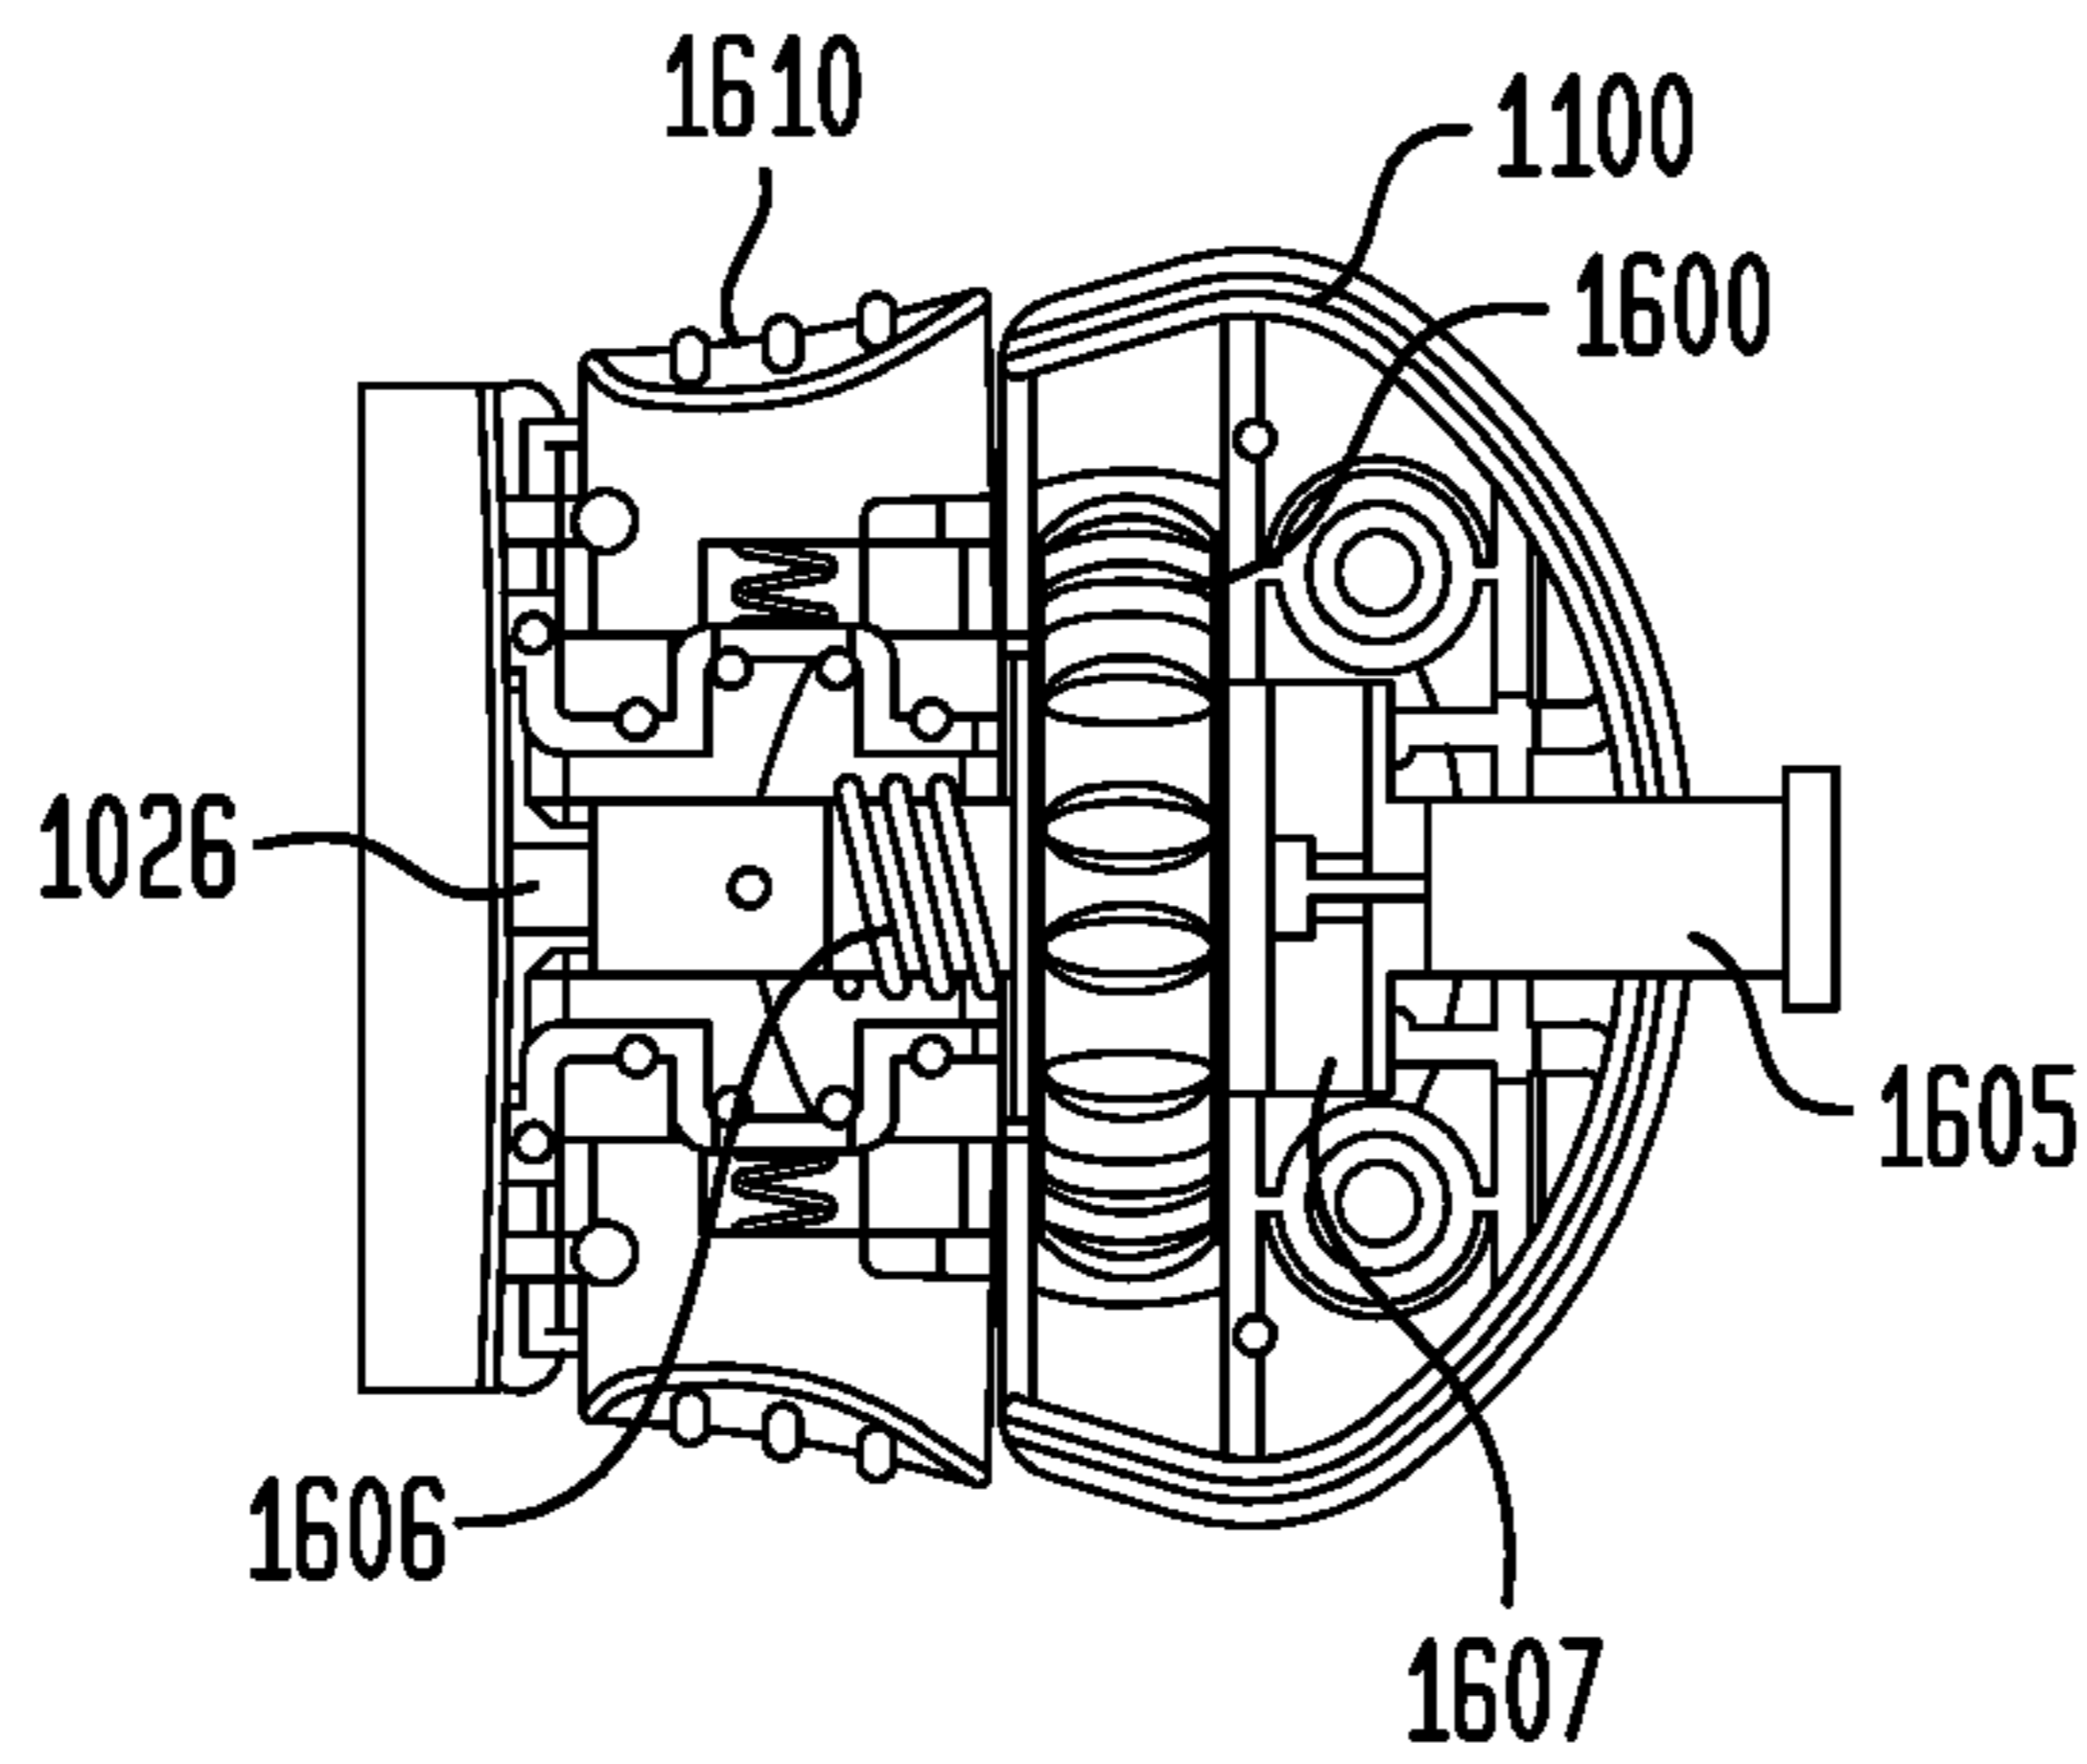


FIG. 8C

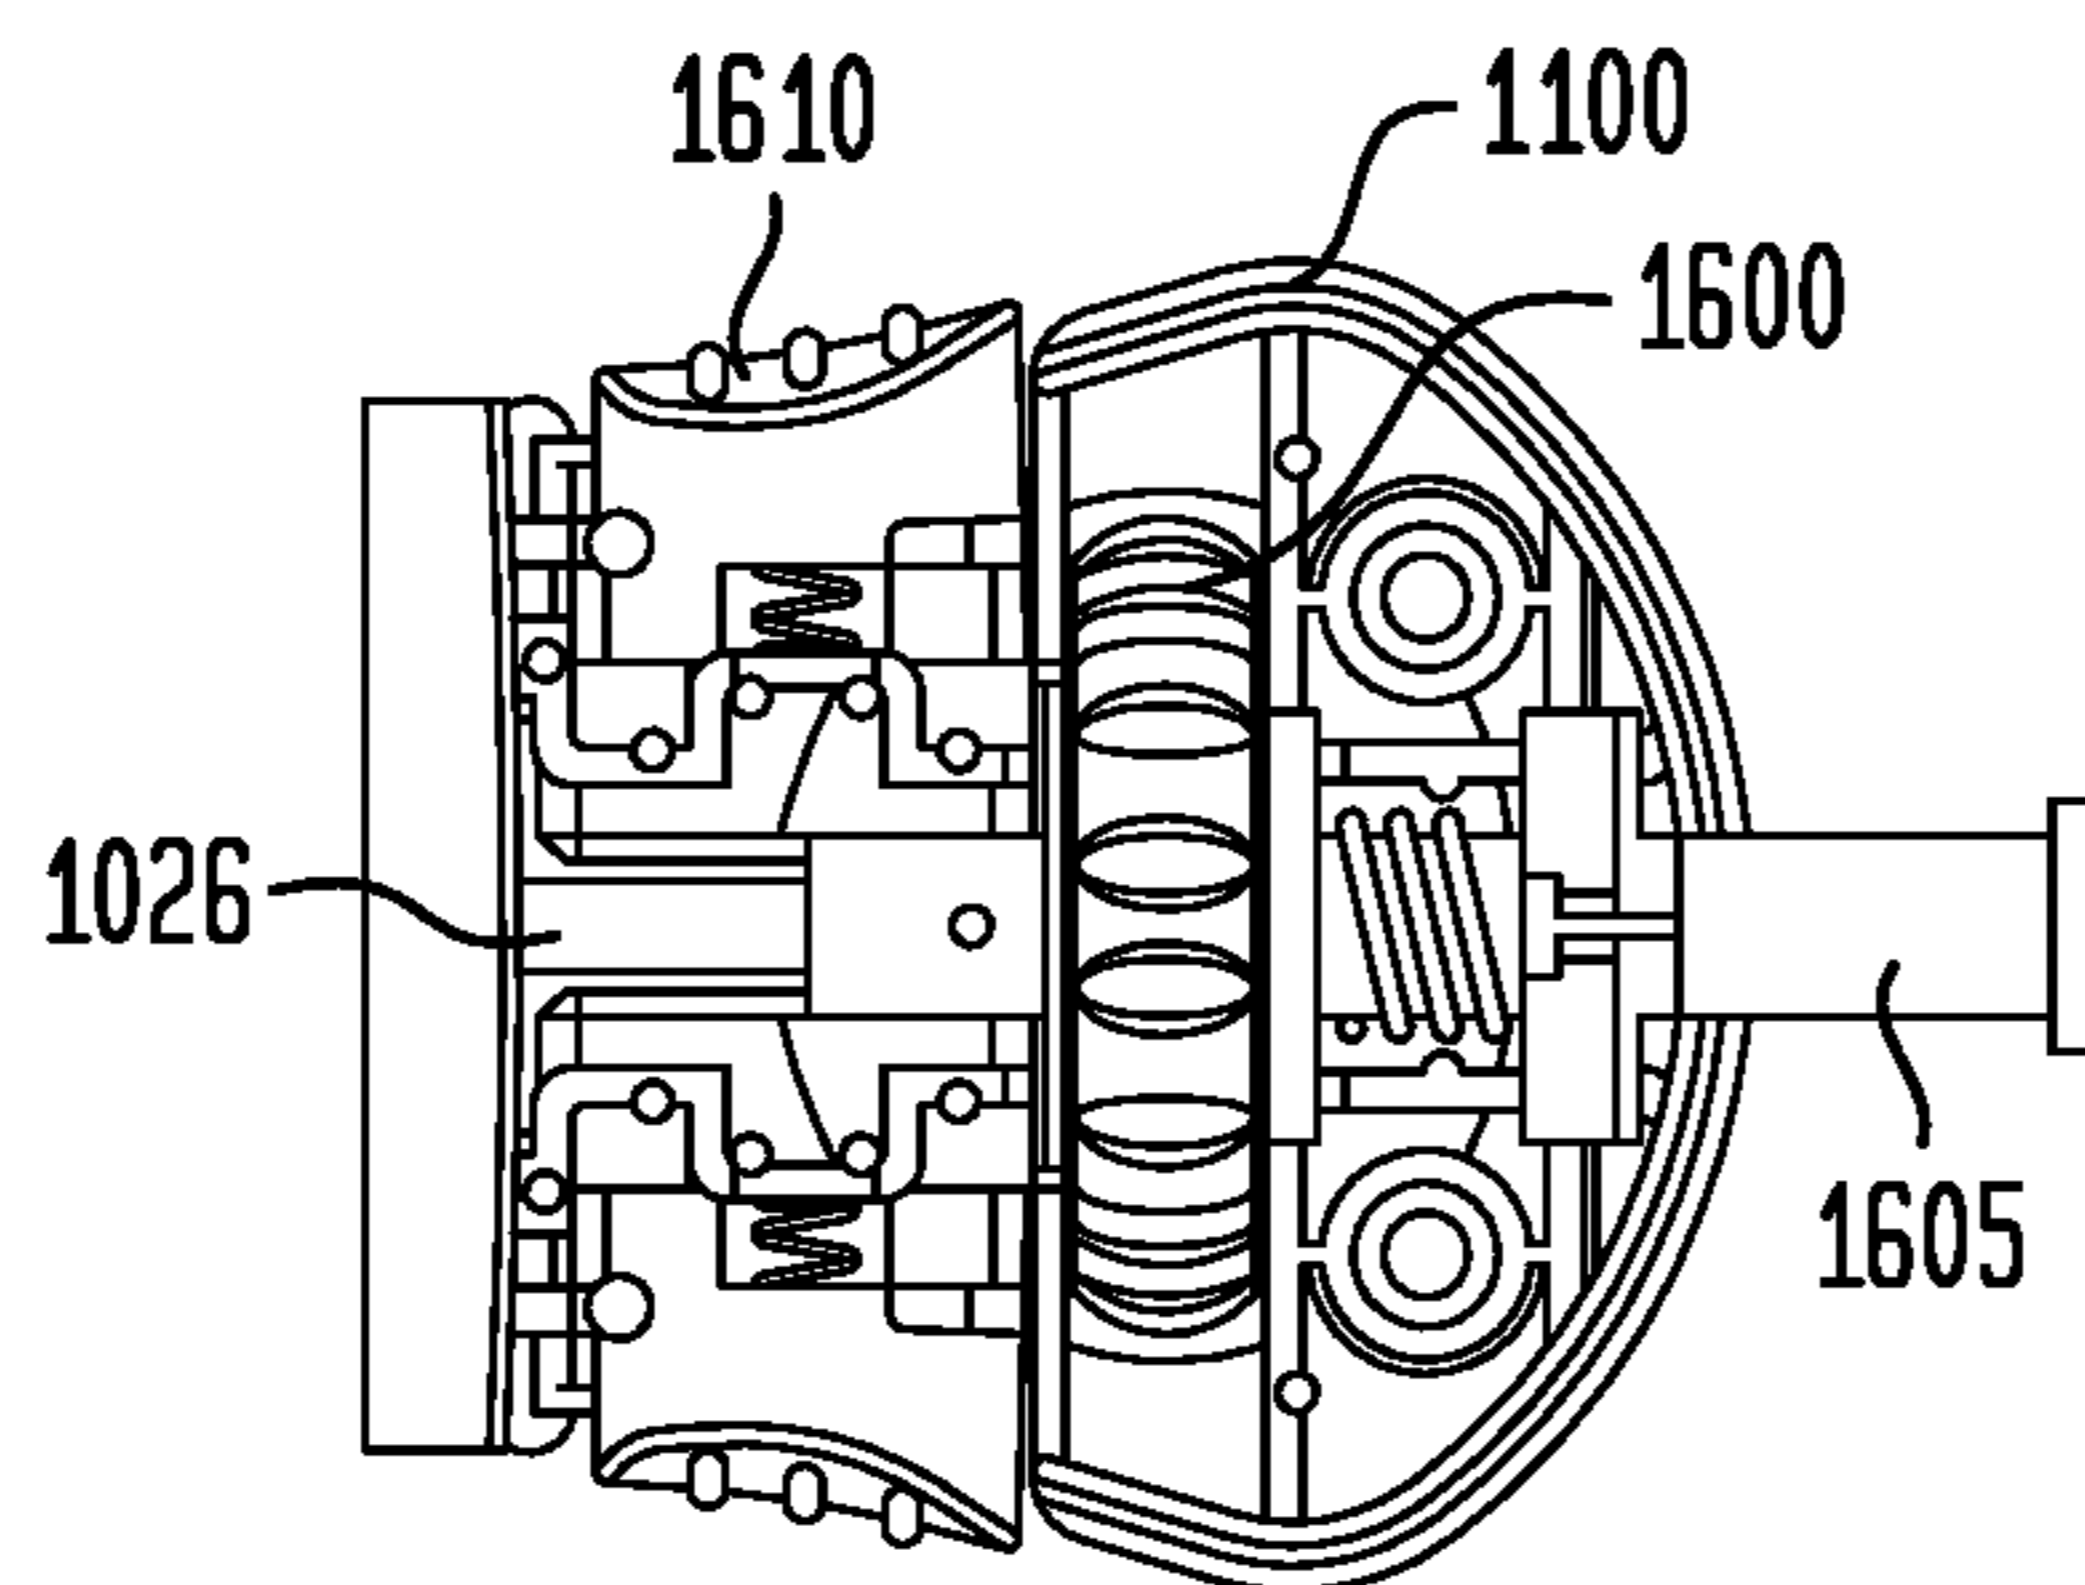


FIG. 9A

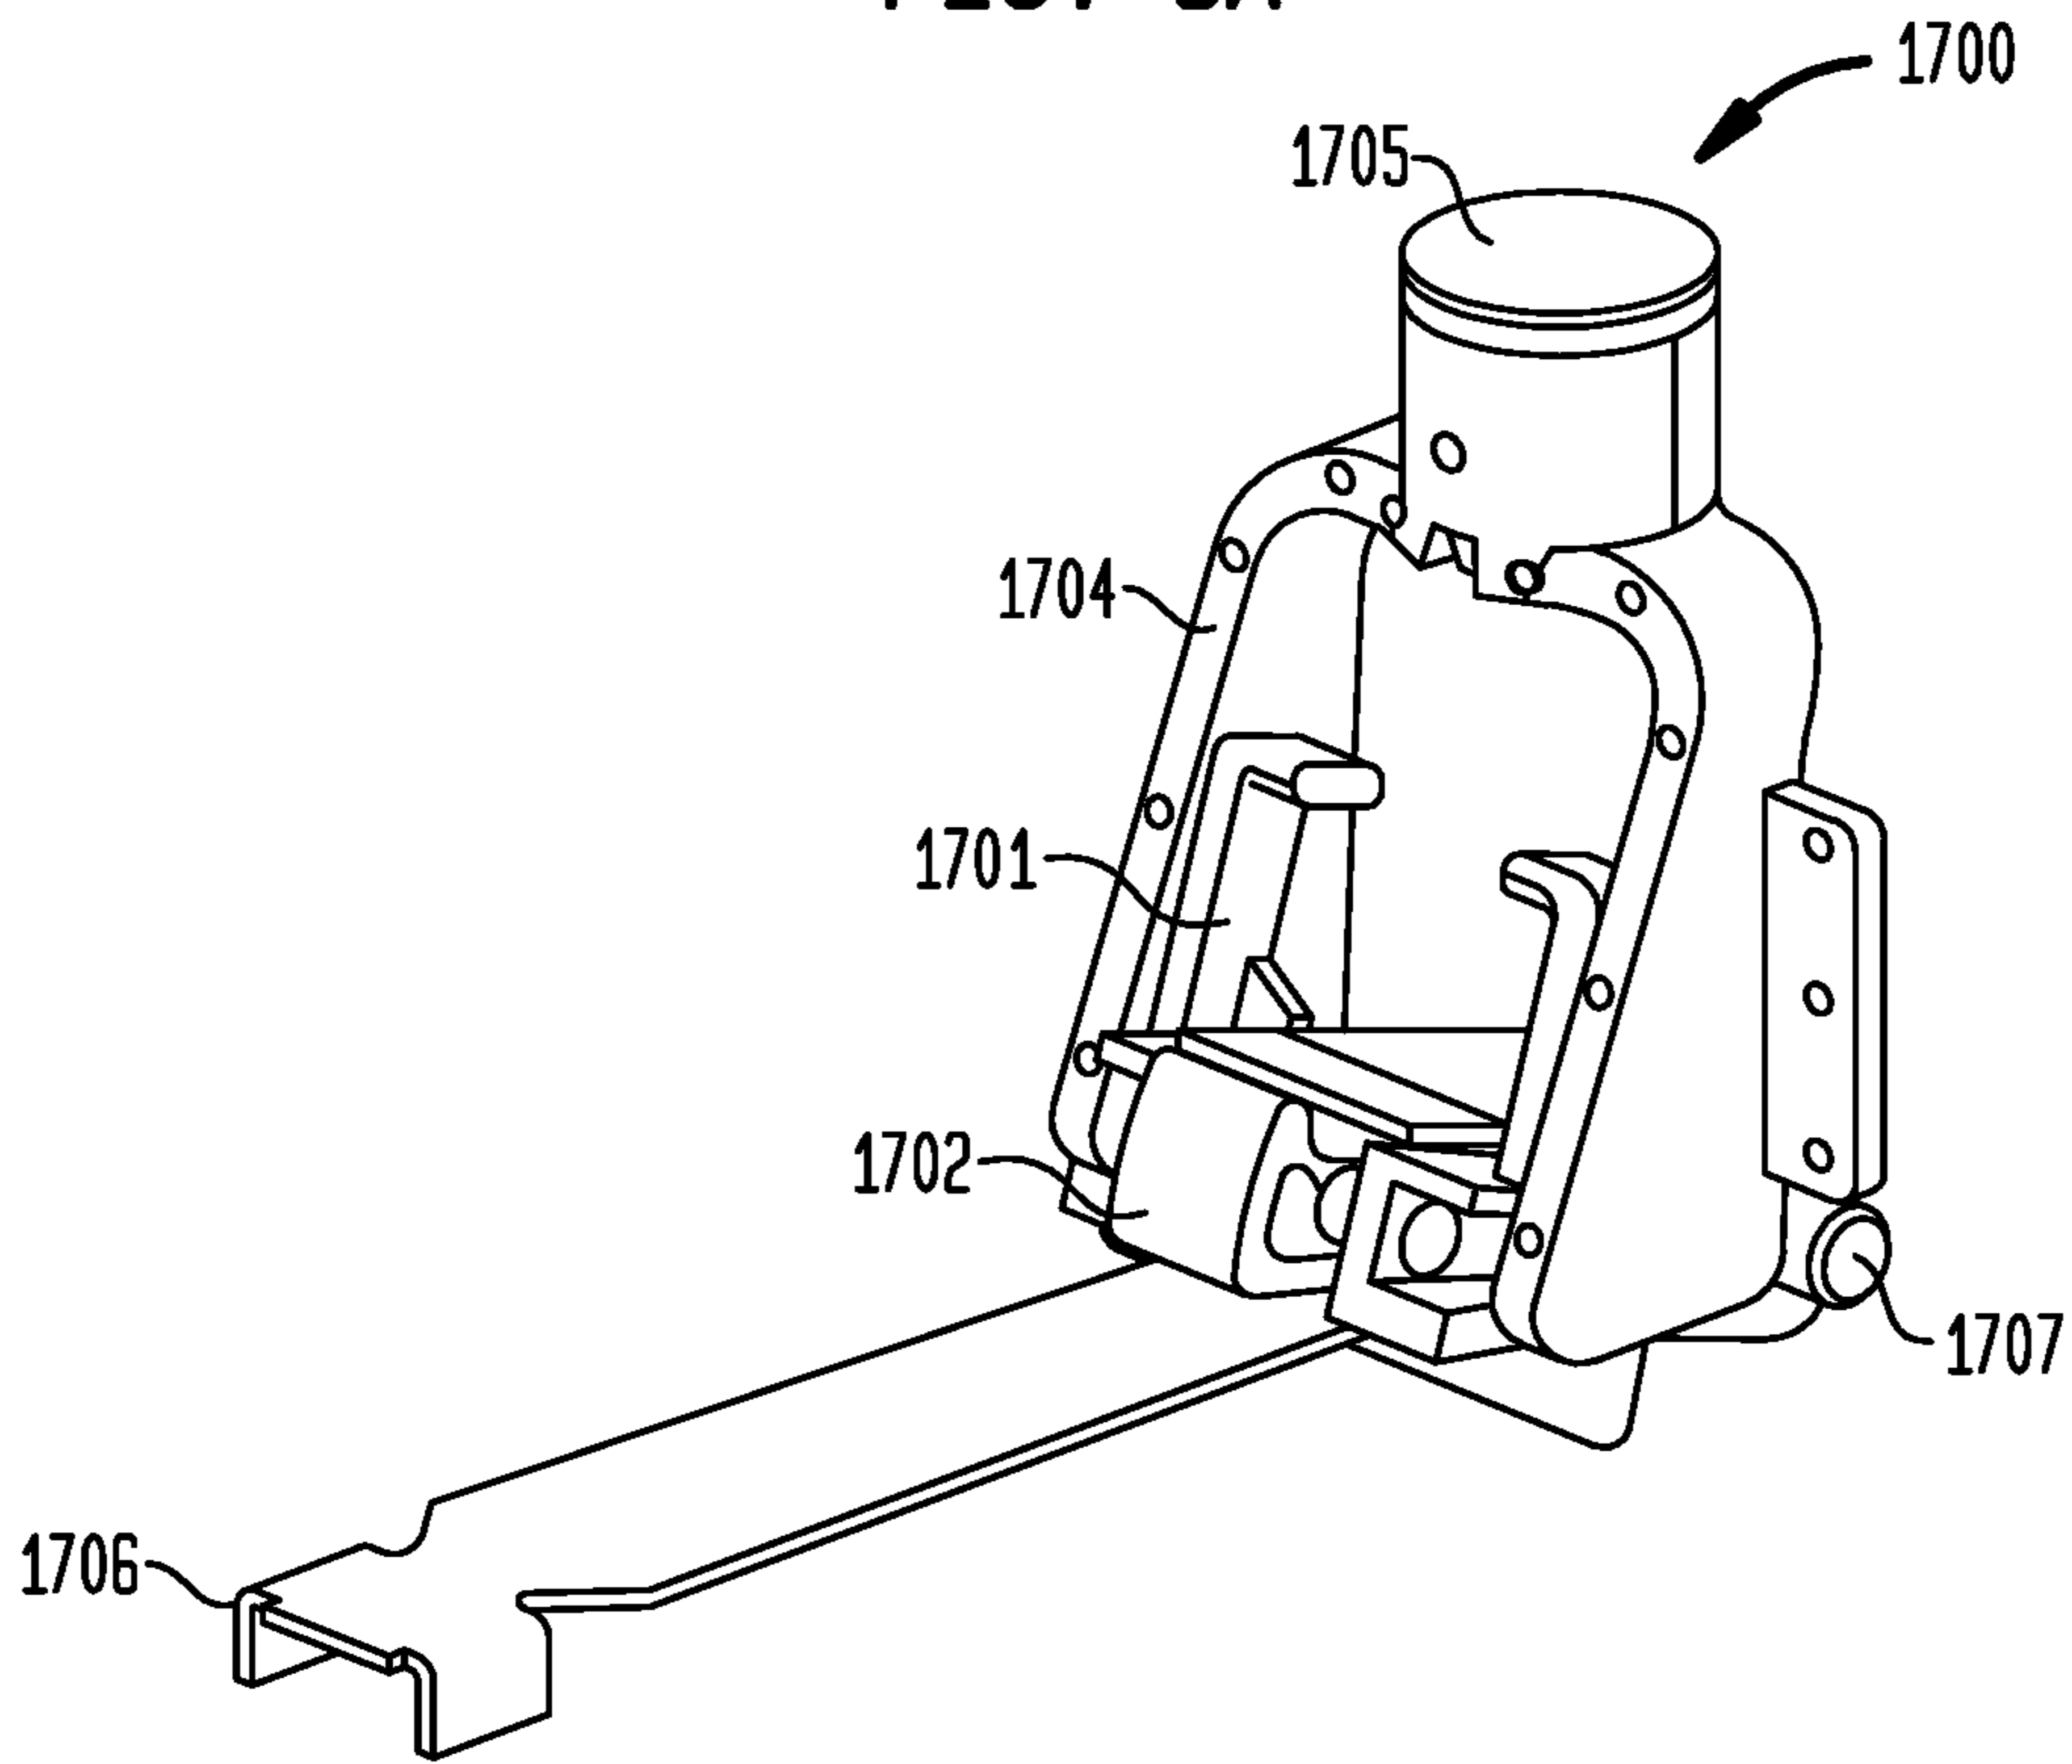


FIG. 9B

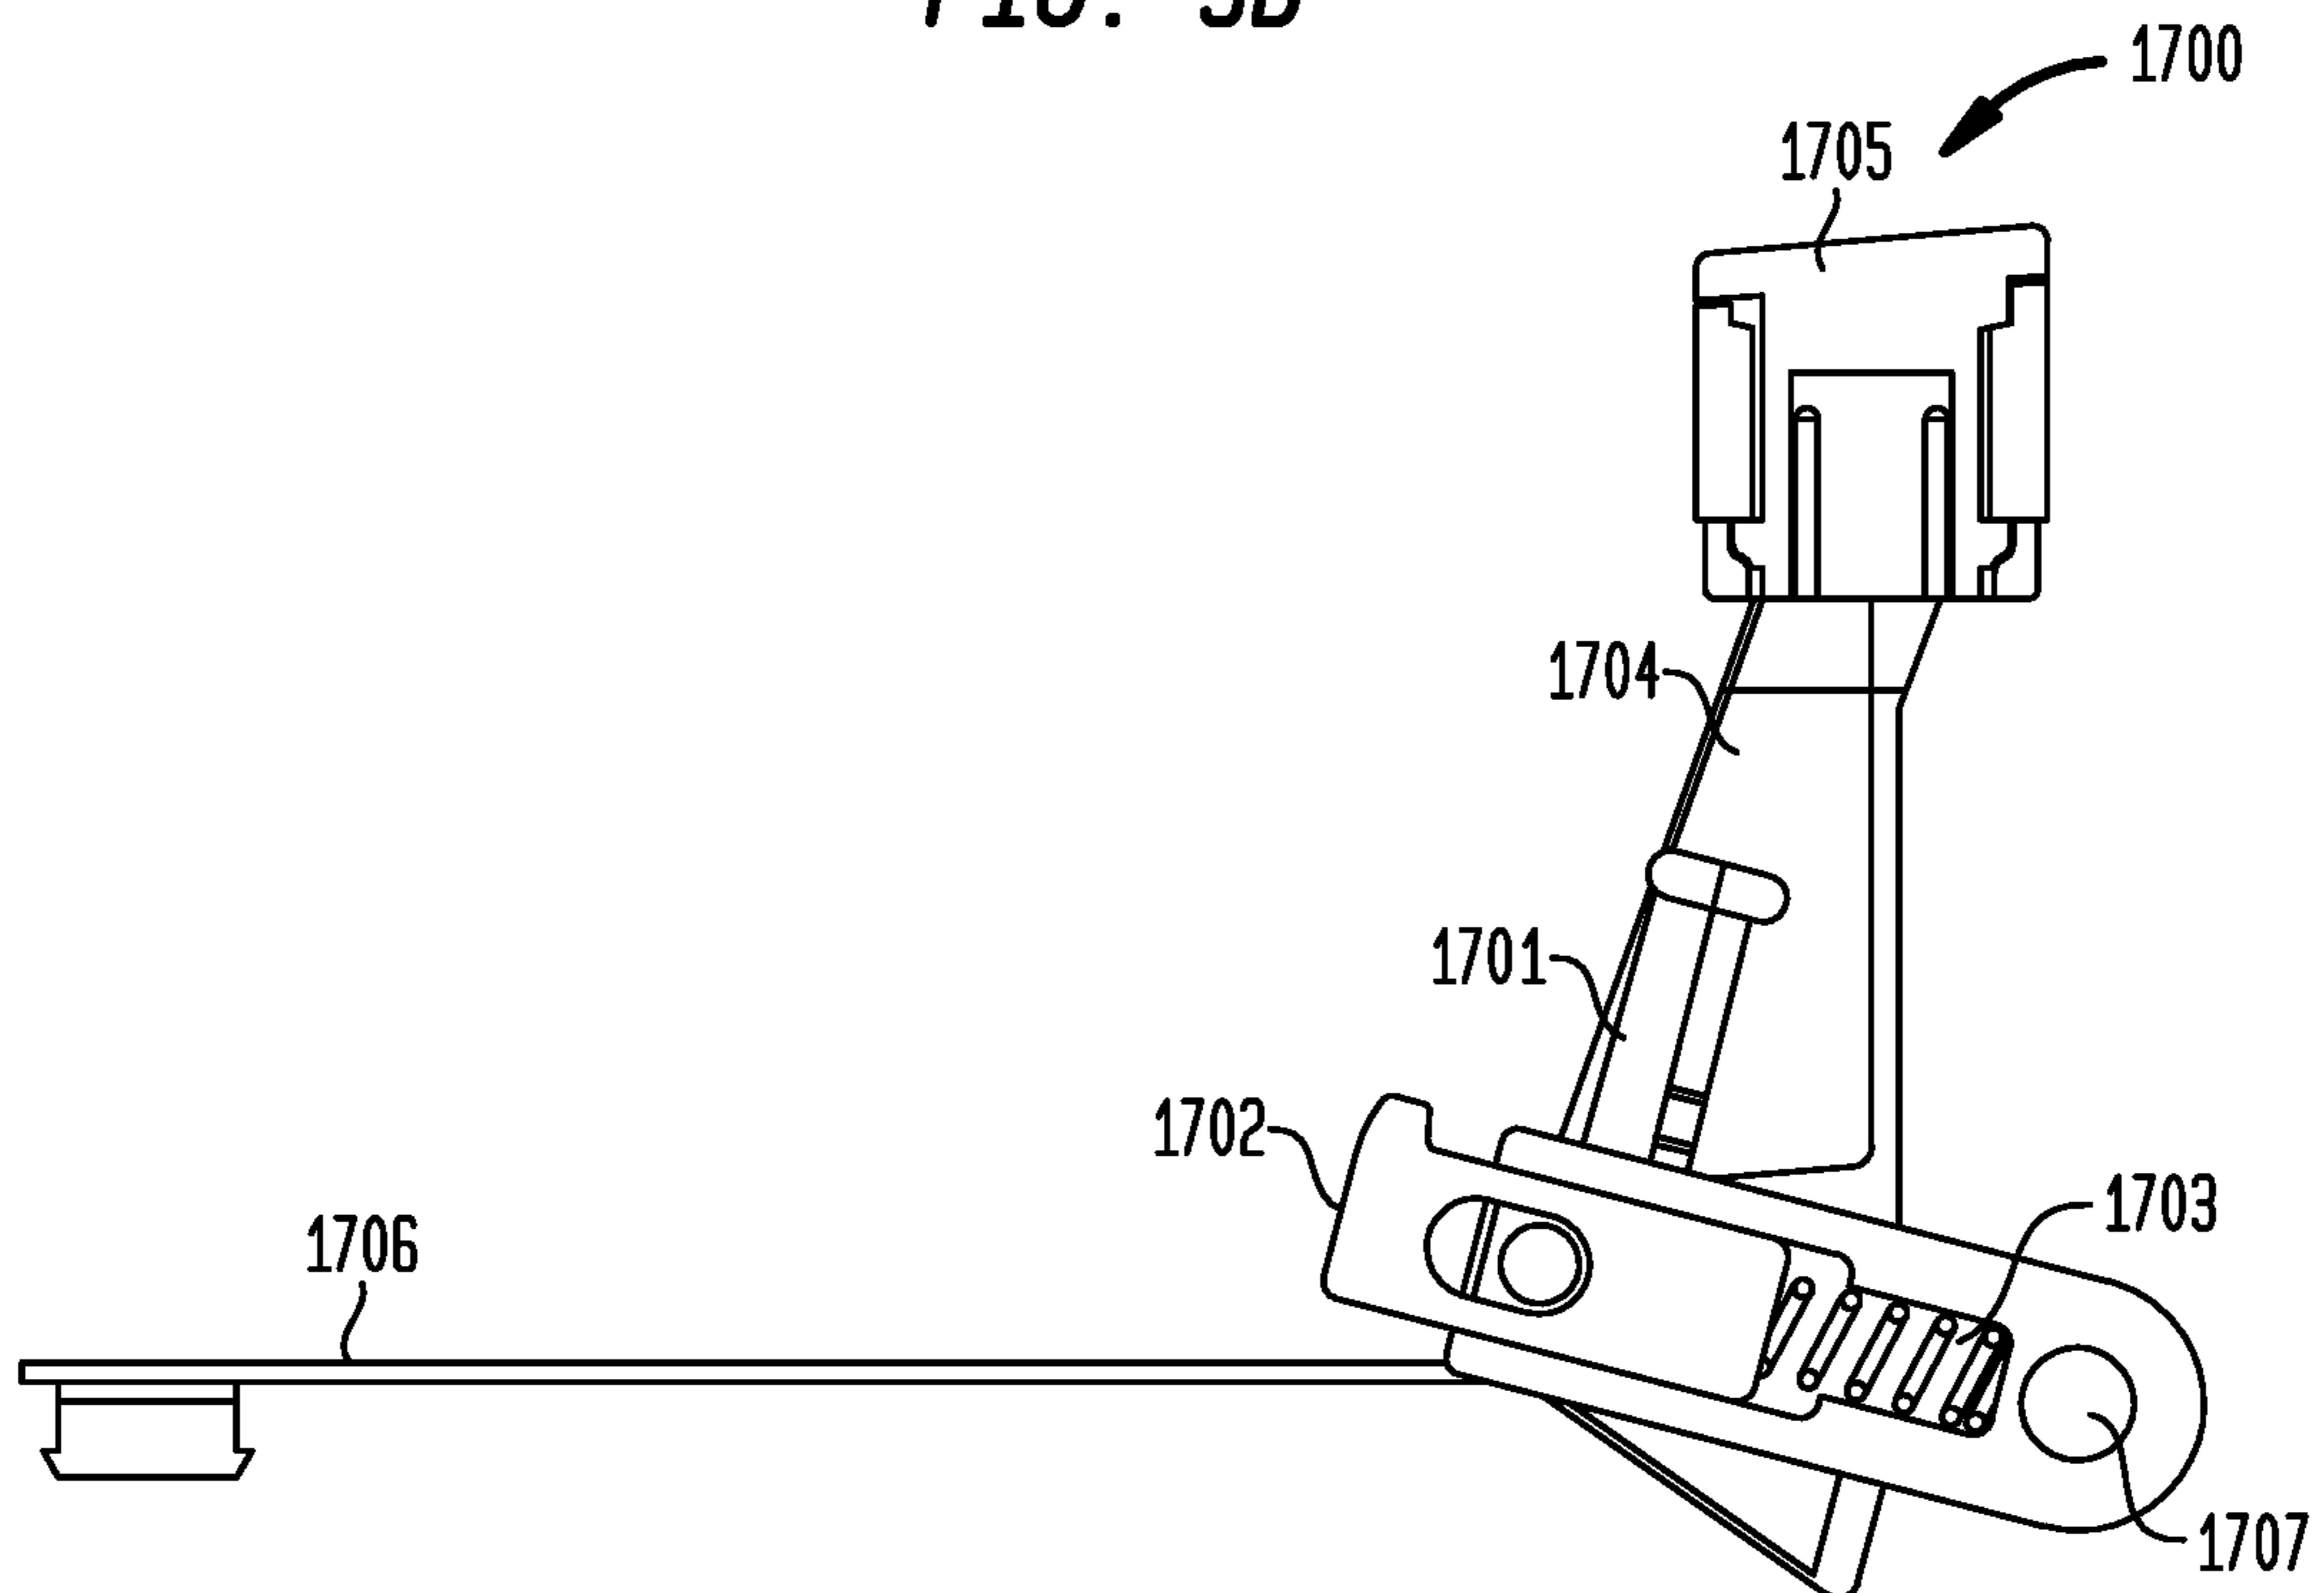


FIG. 9C



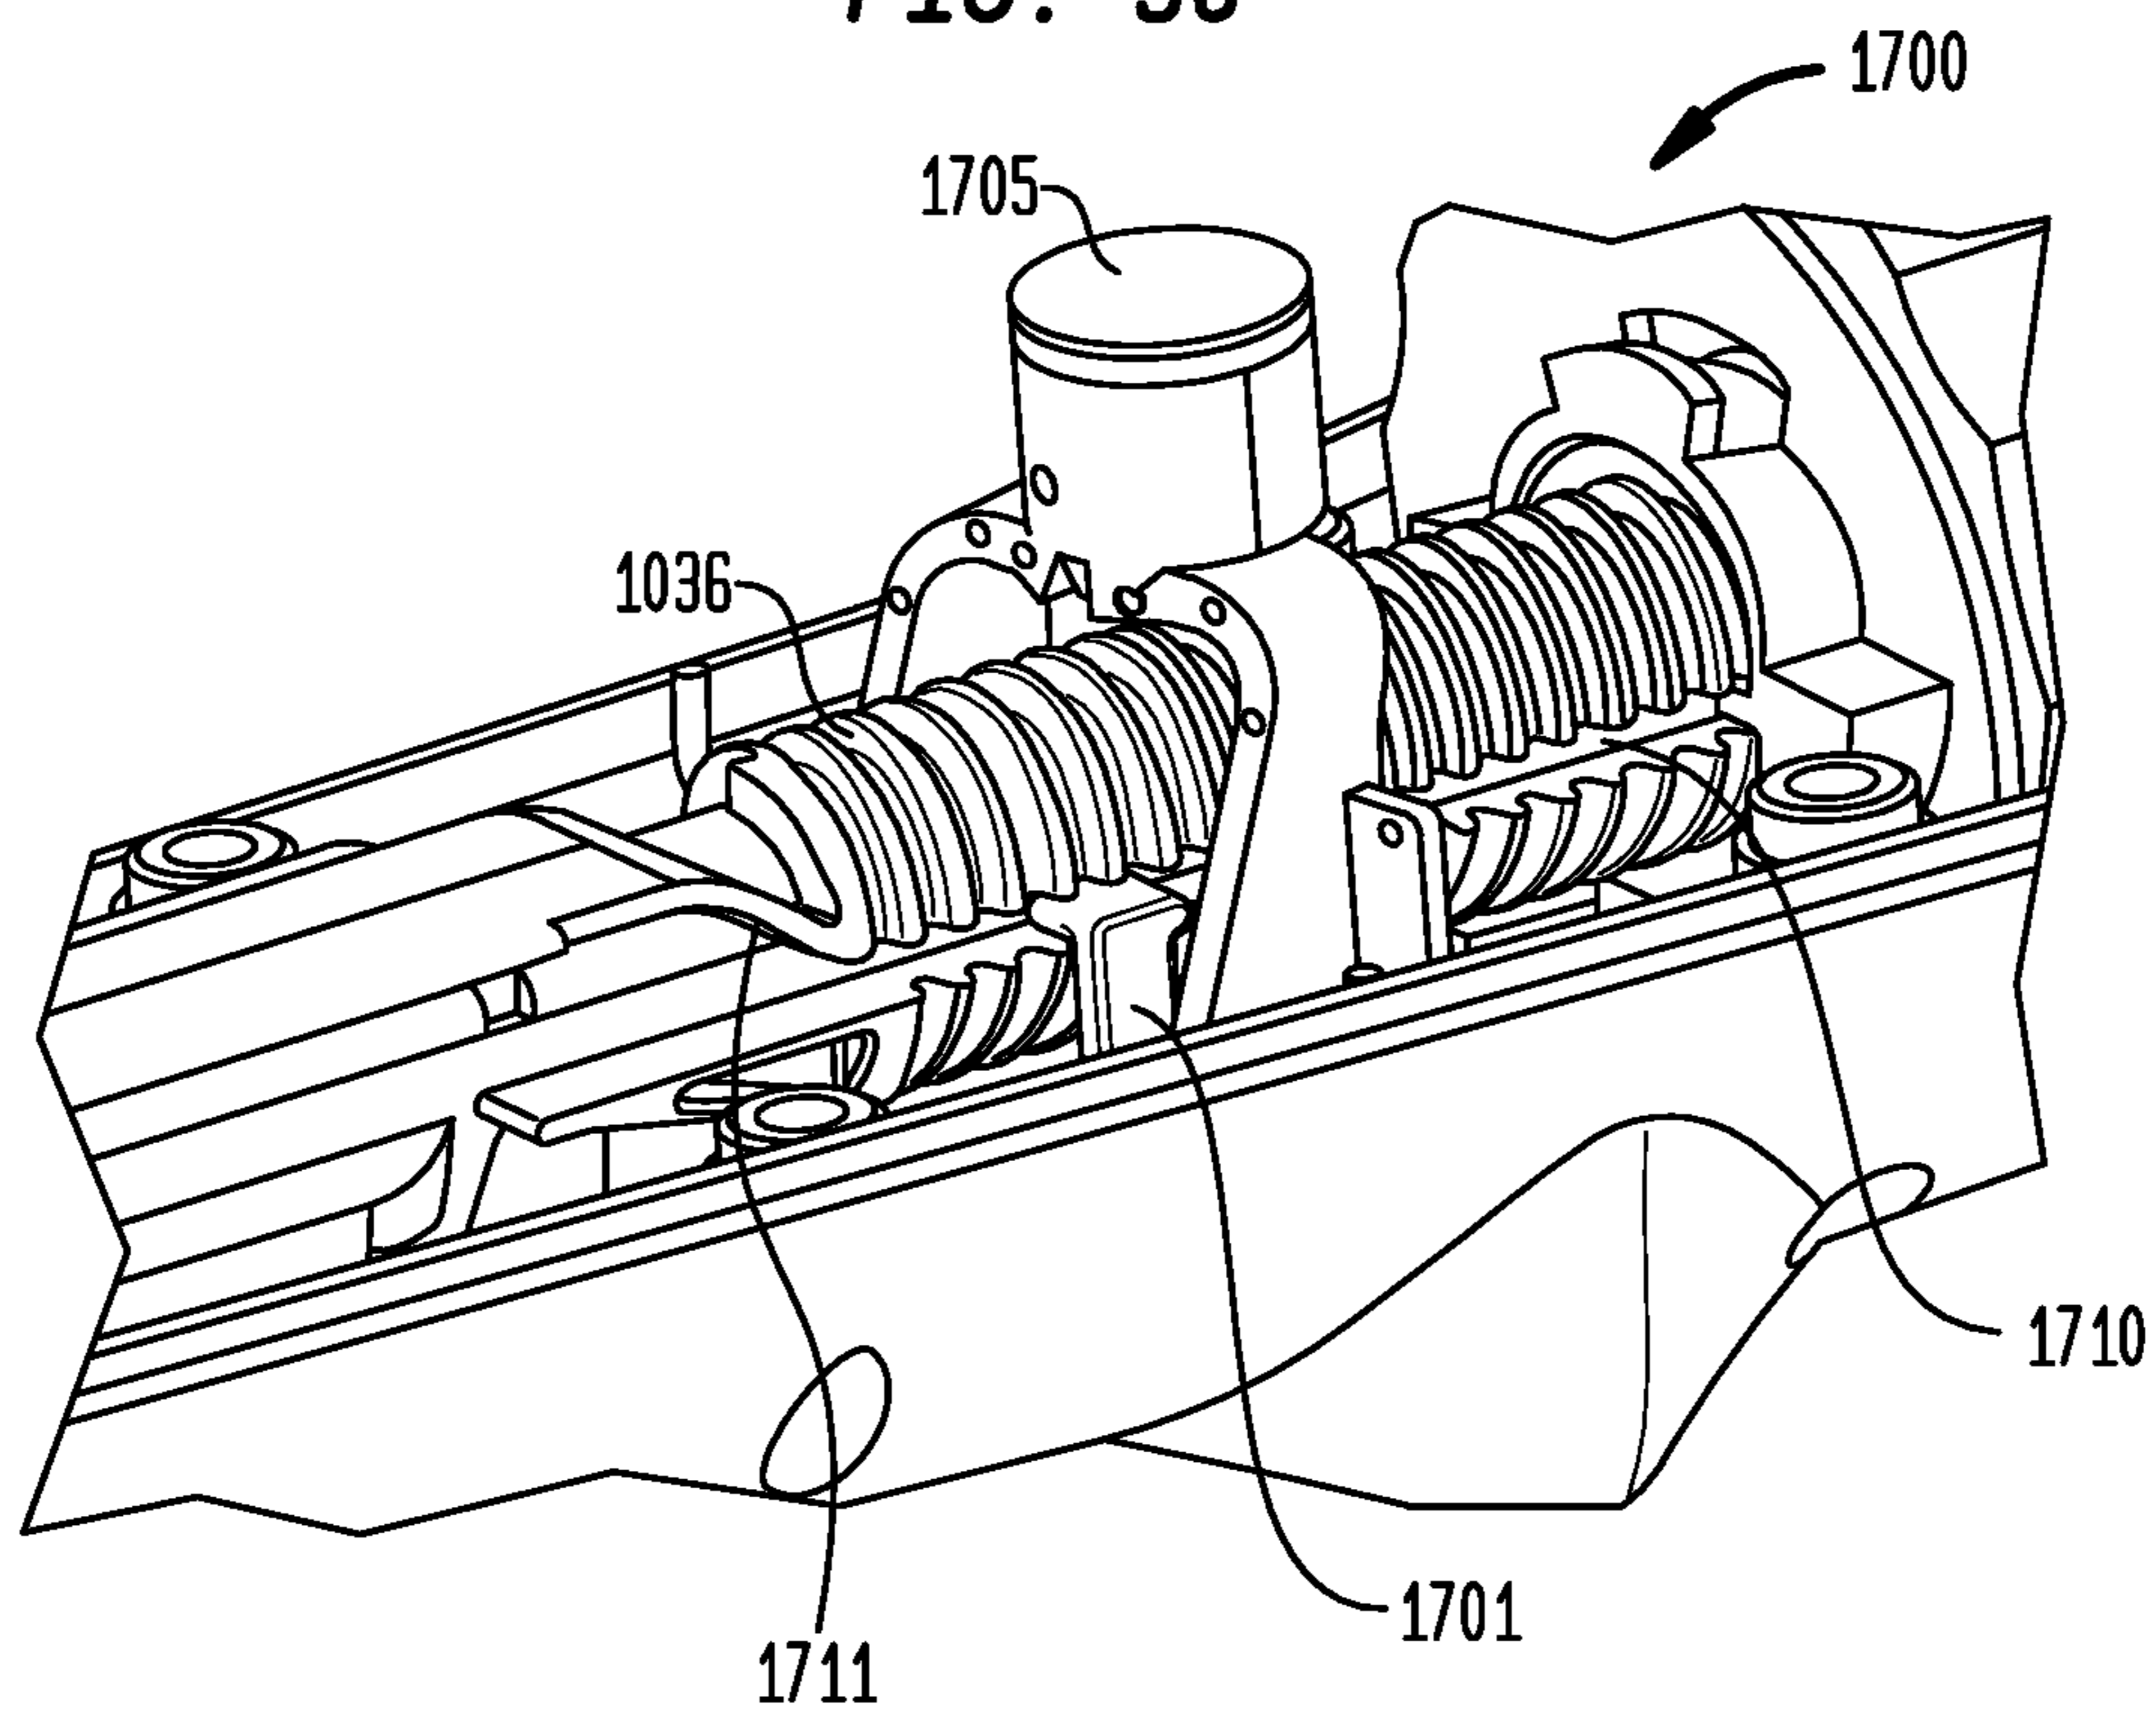



FIG. 9D

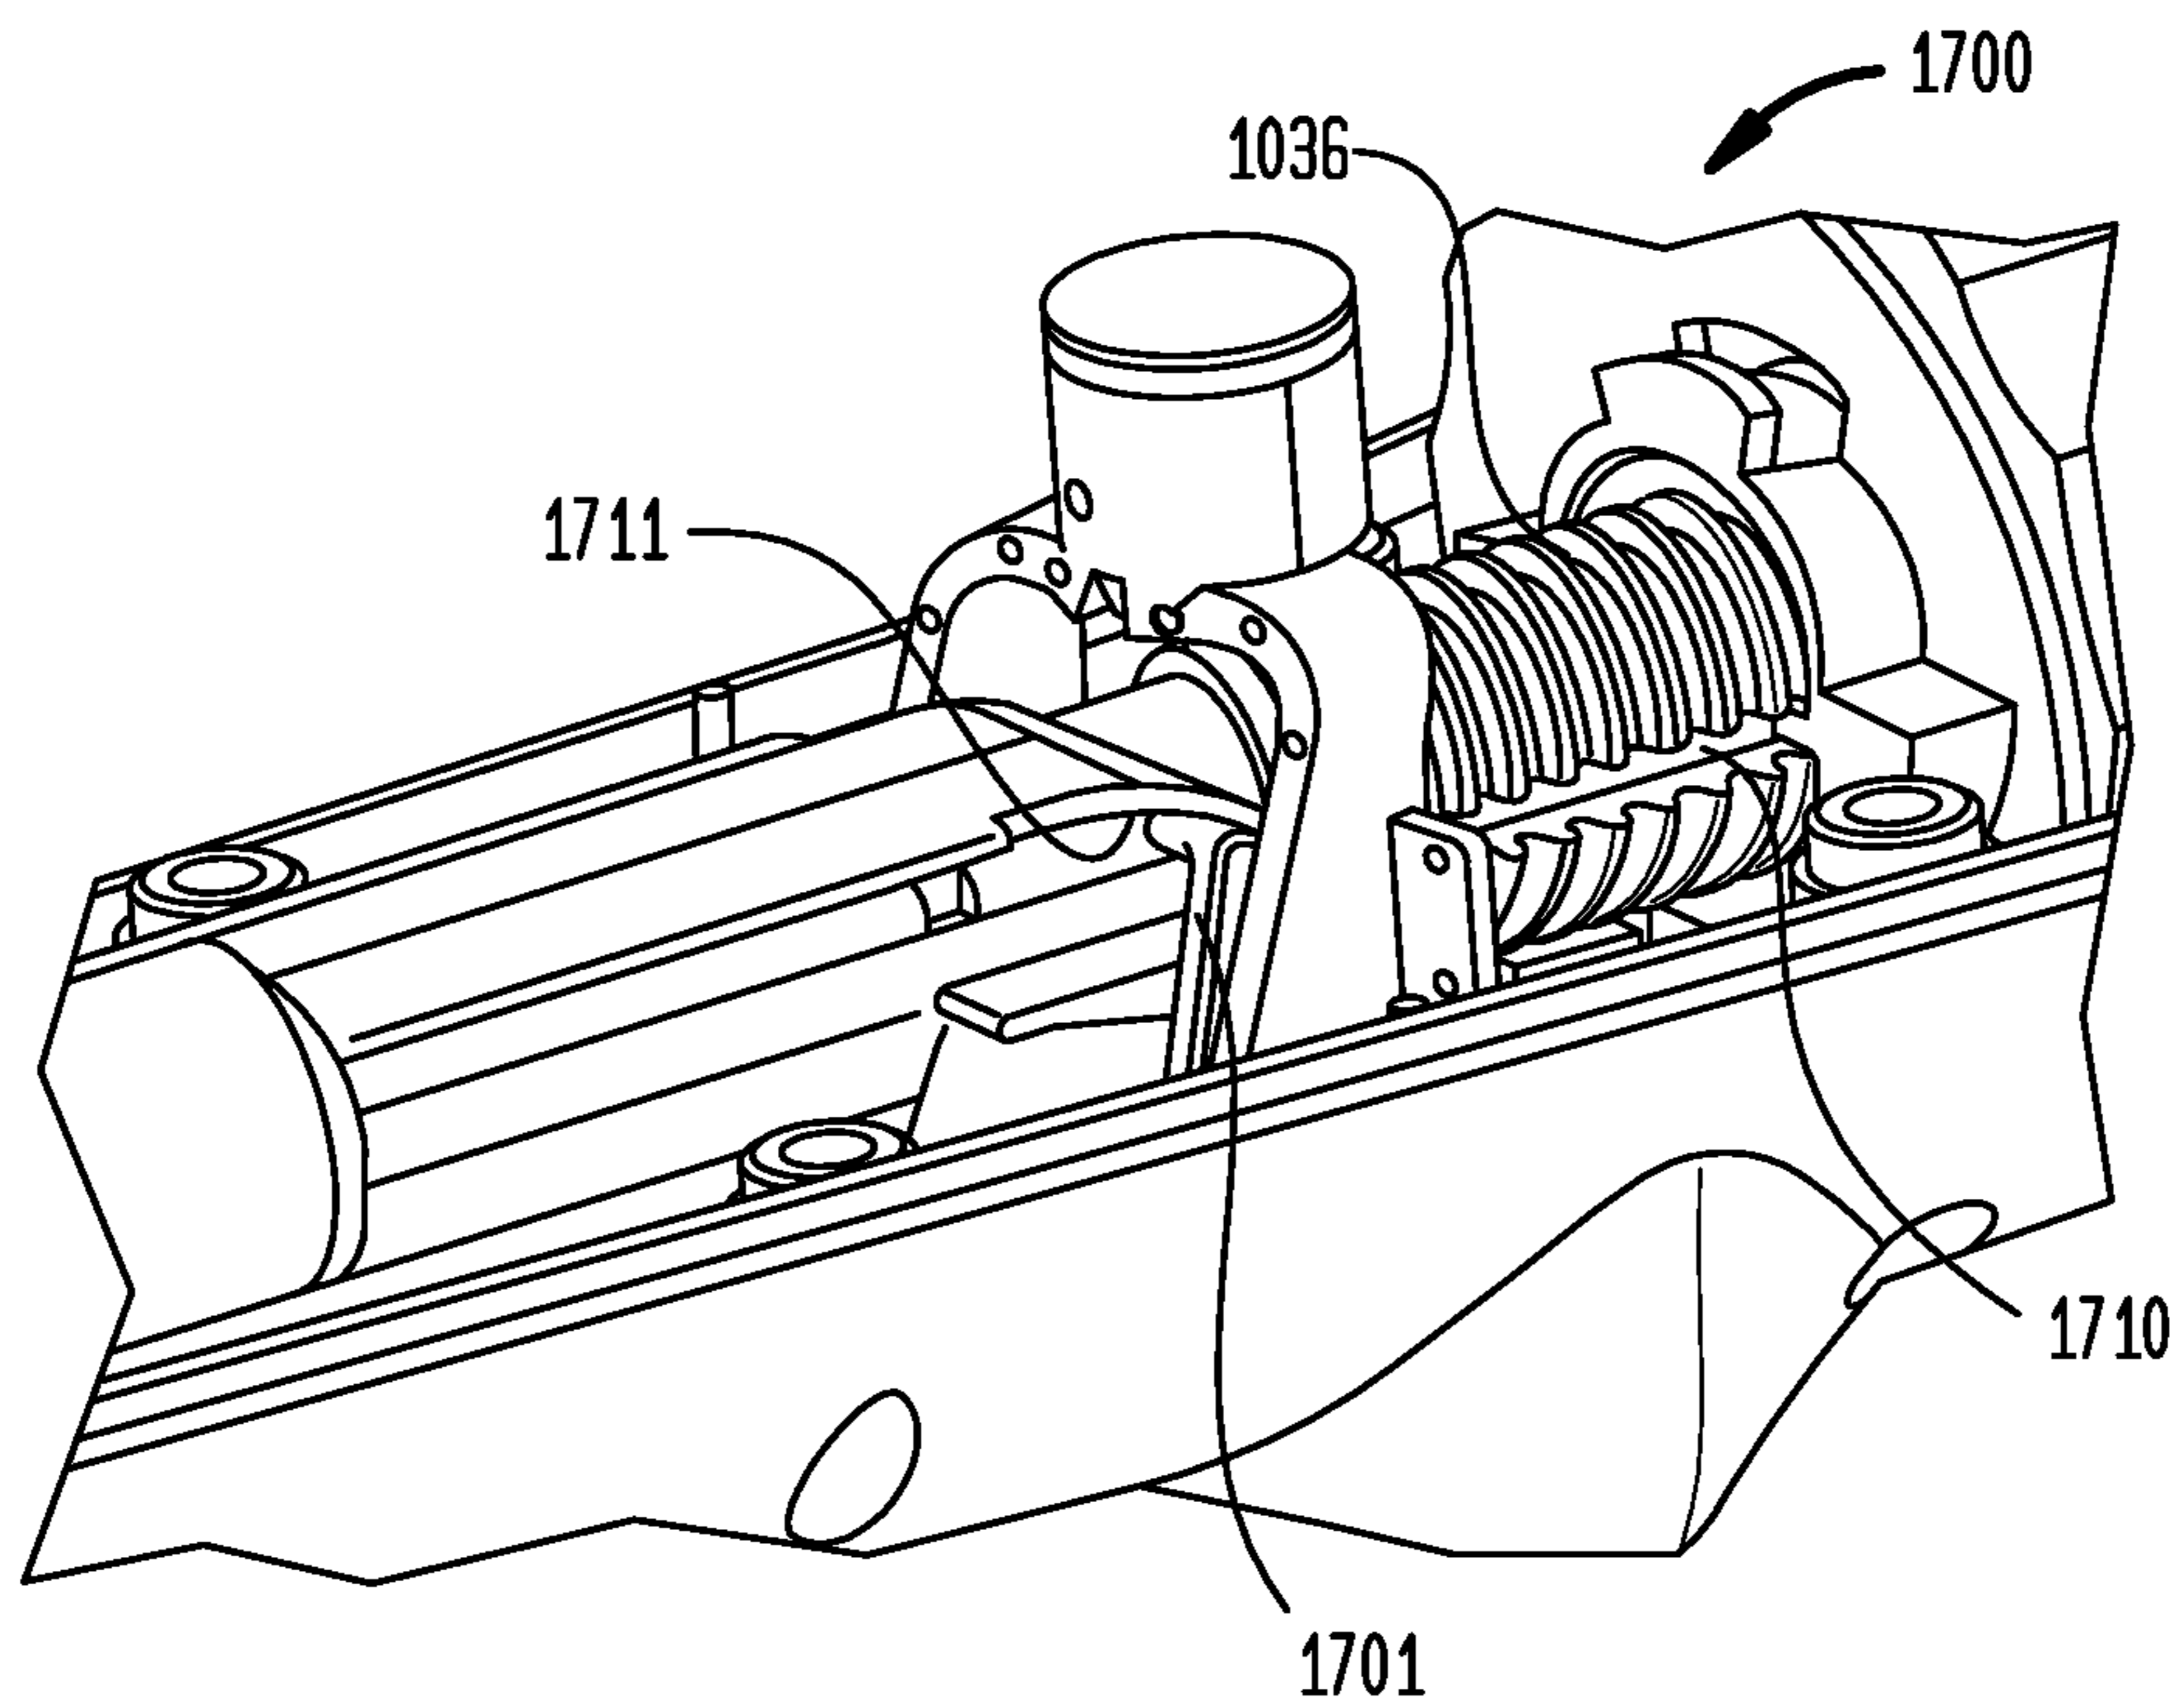

**FIG. 9E**

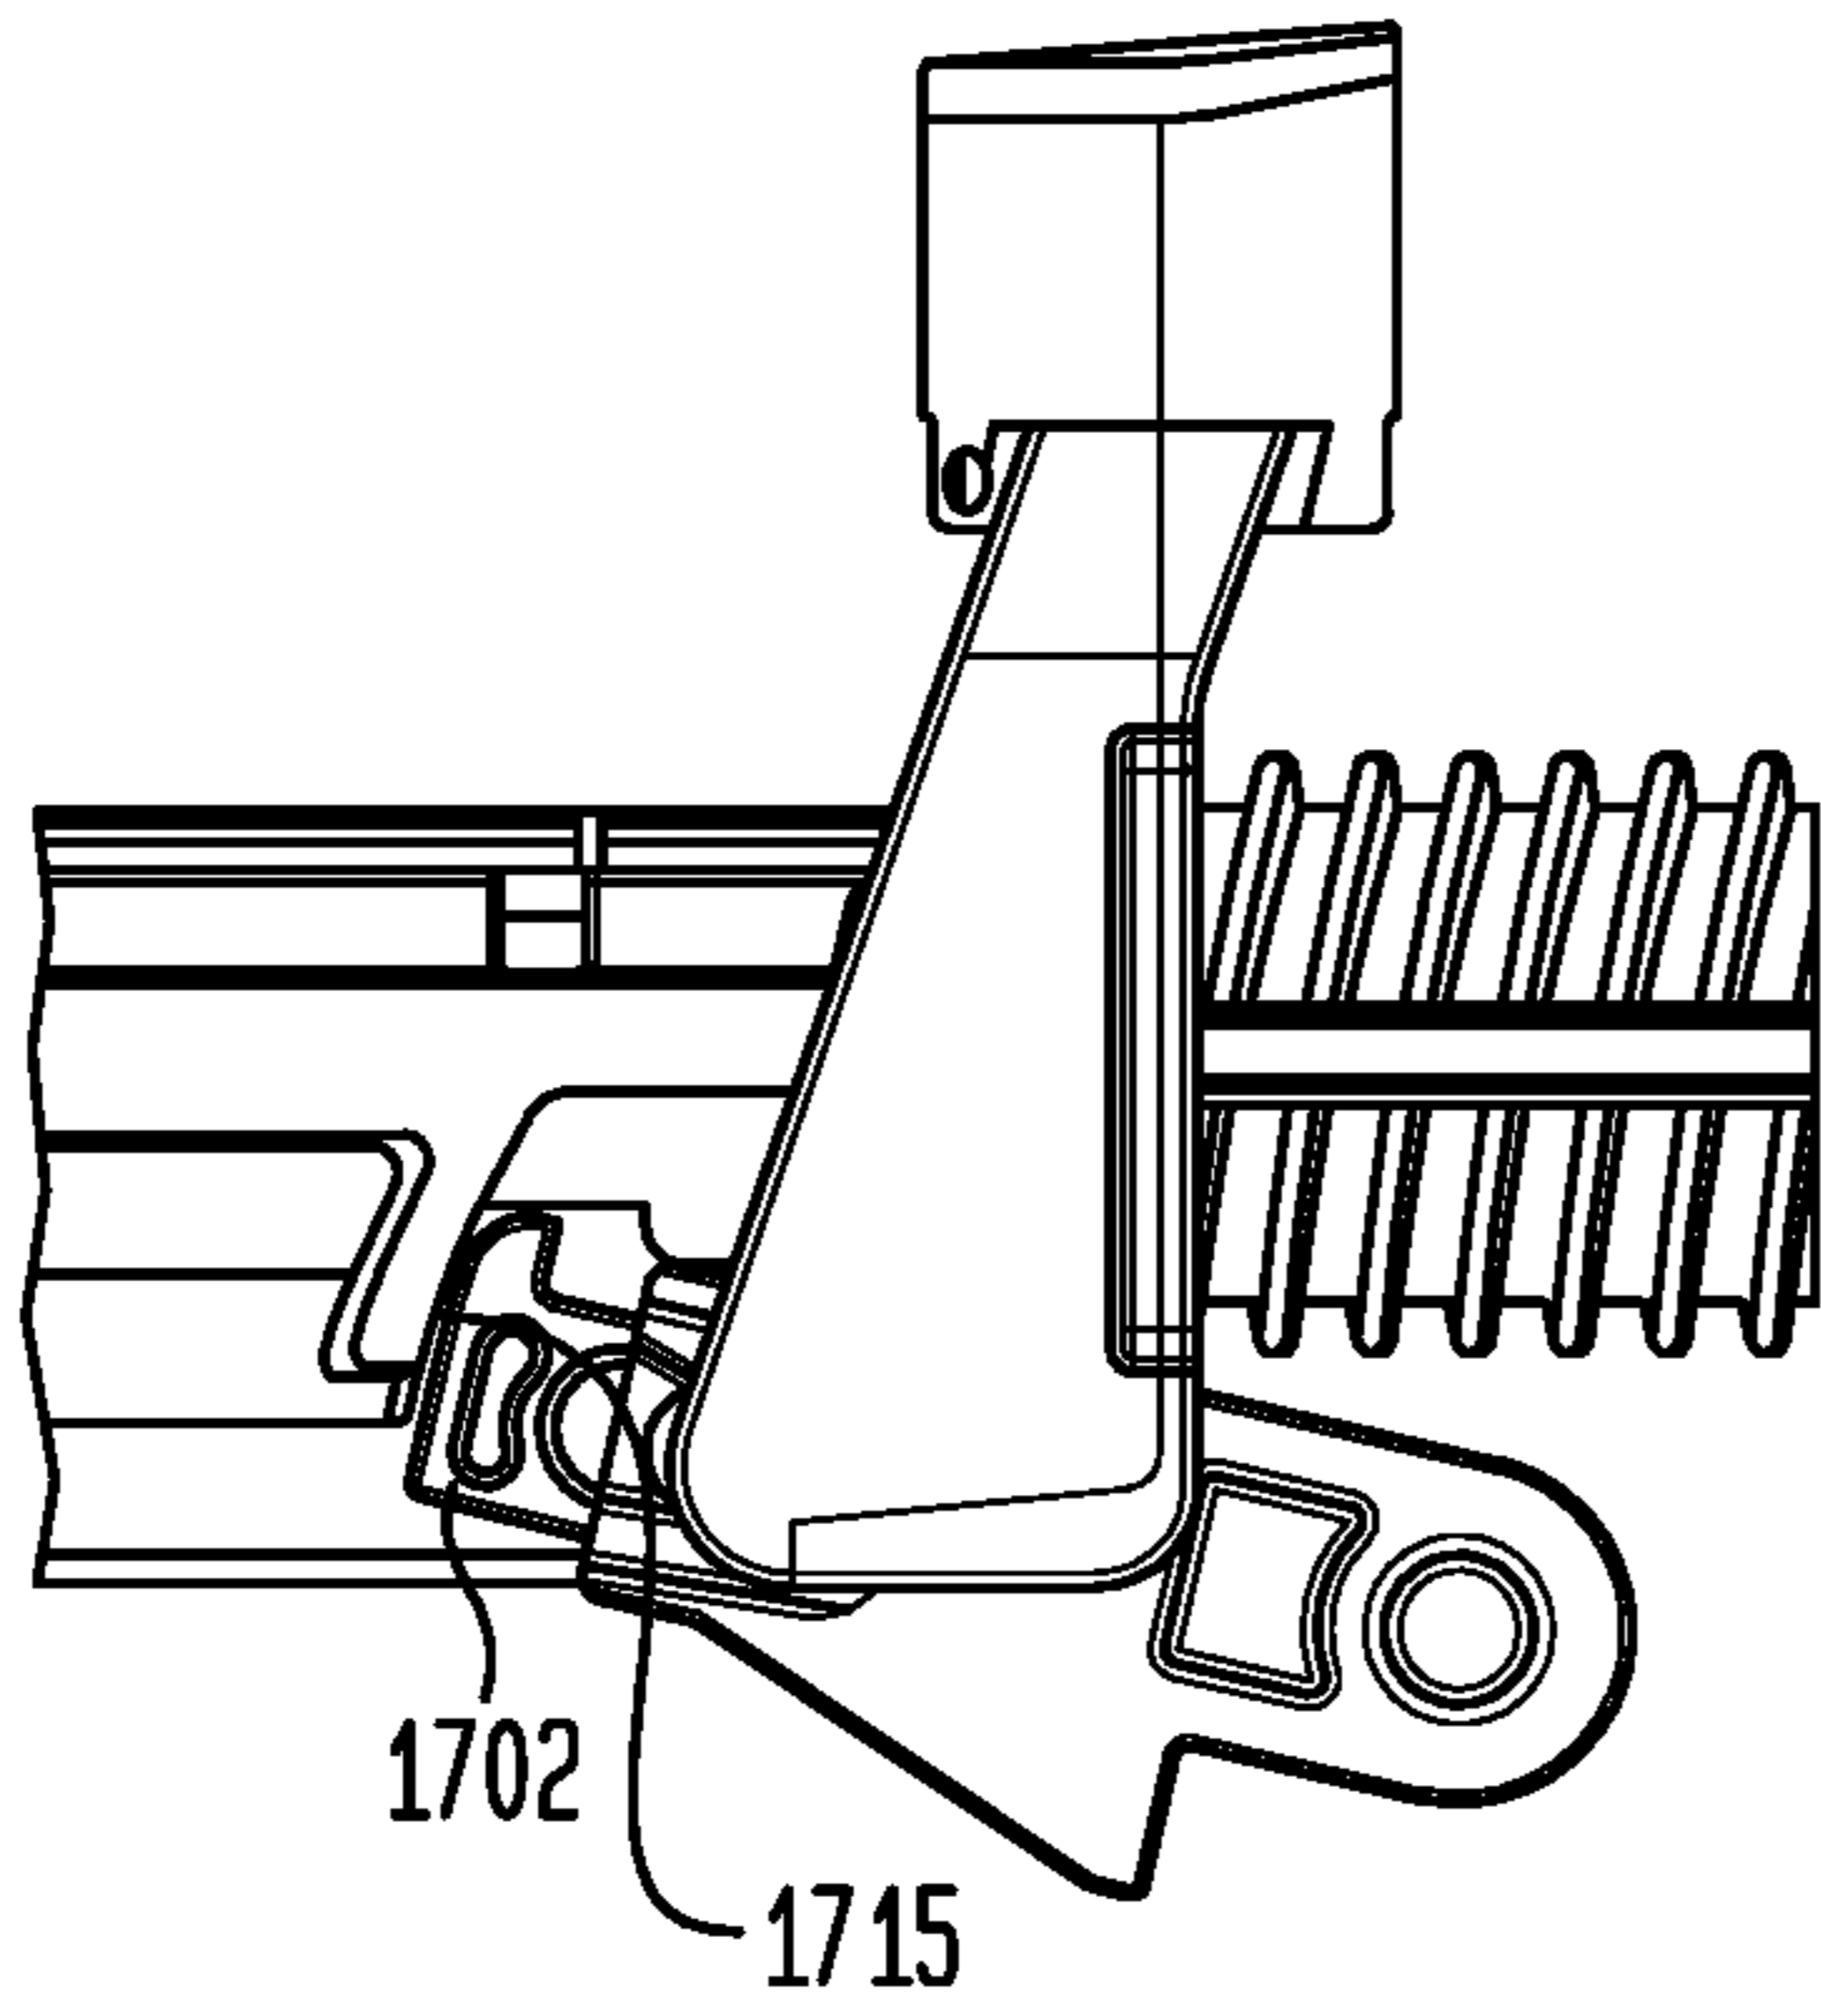

**FIG. 9F**

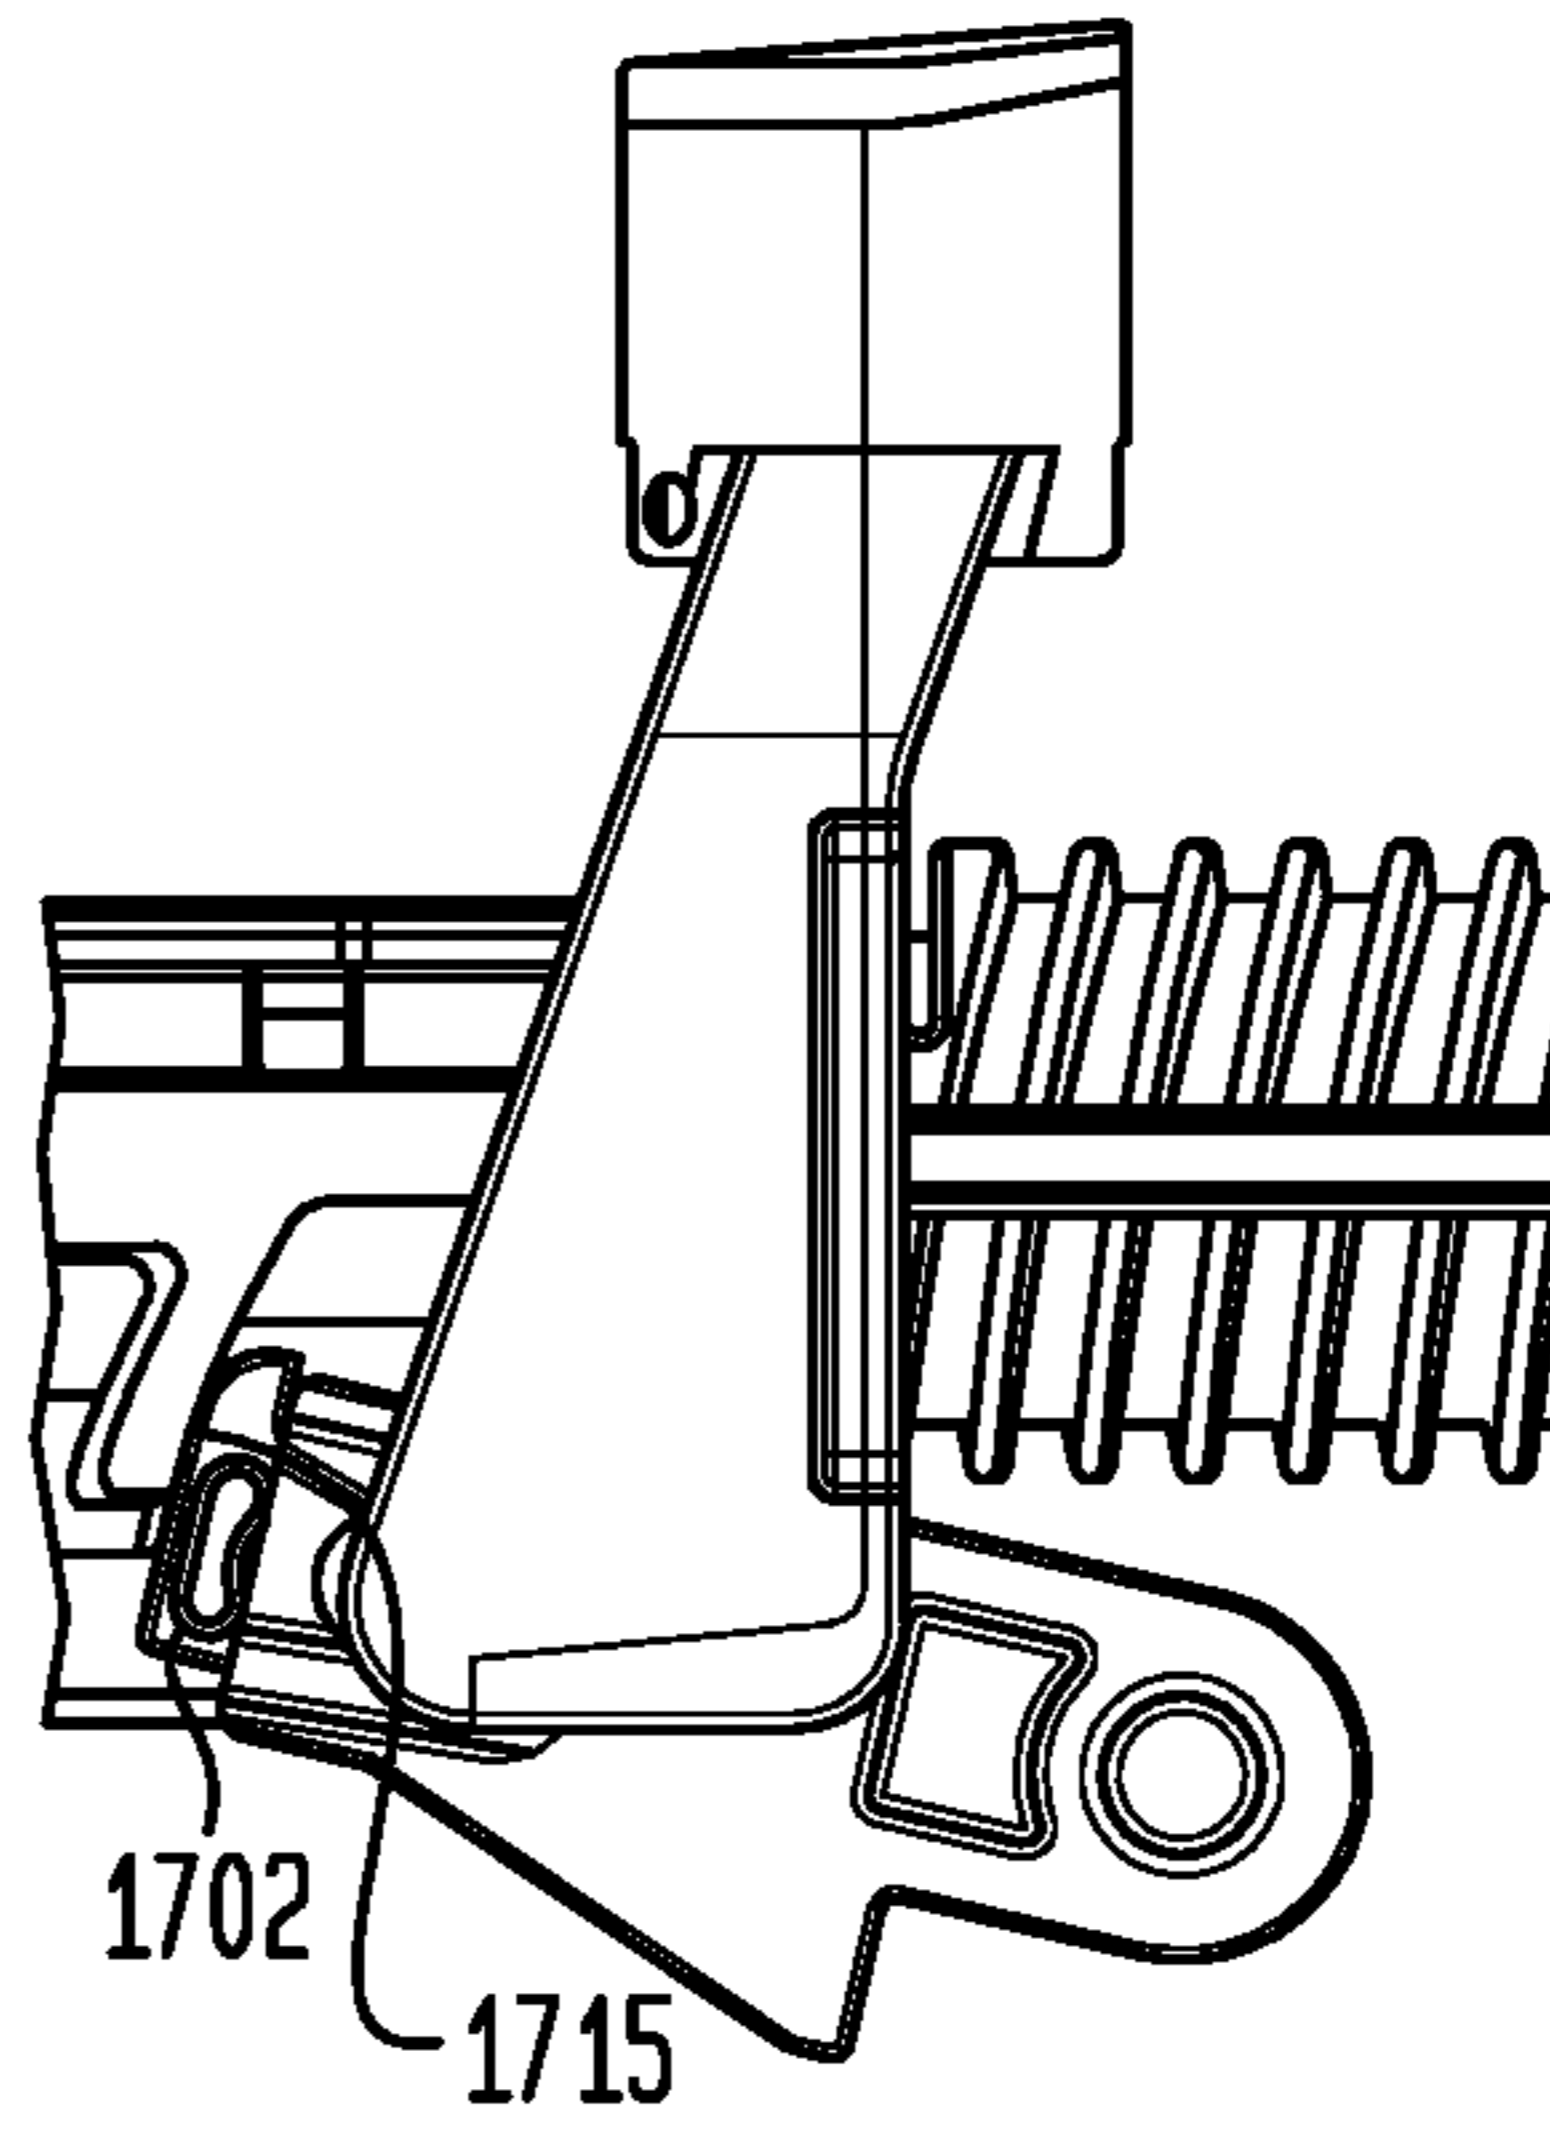

**FIG. 9G**

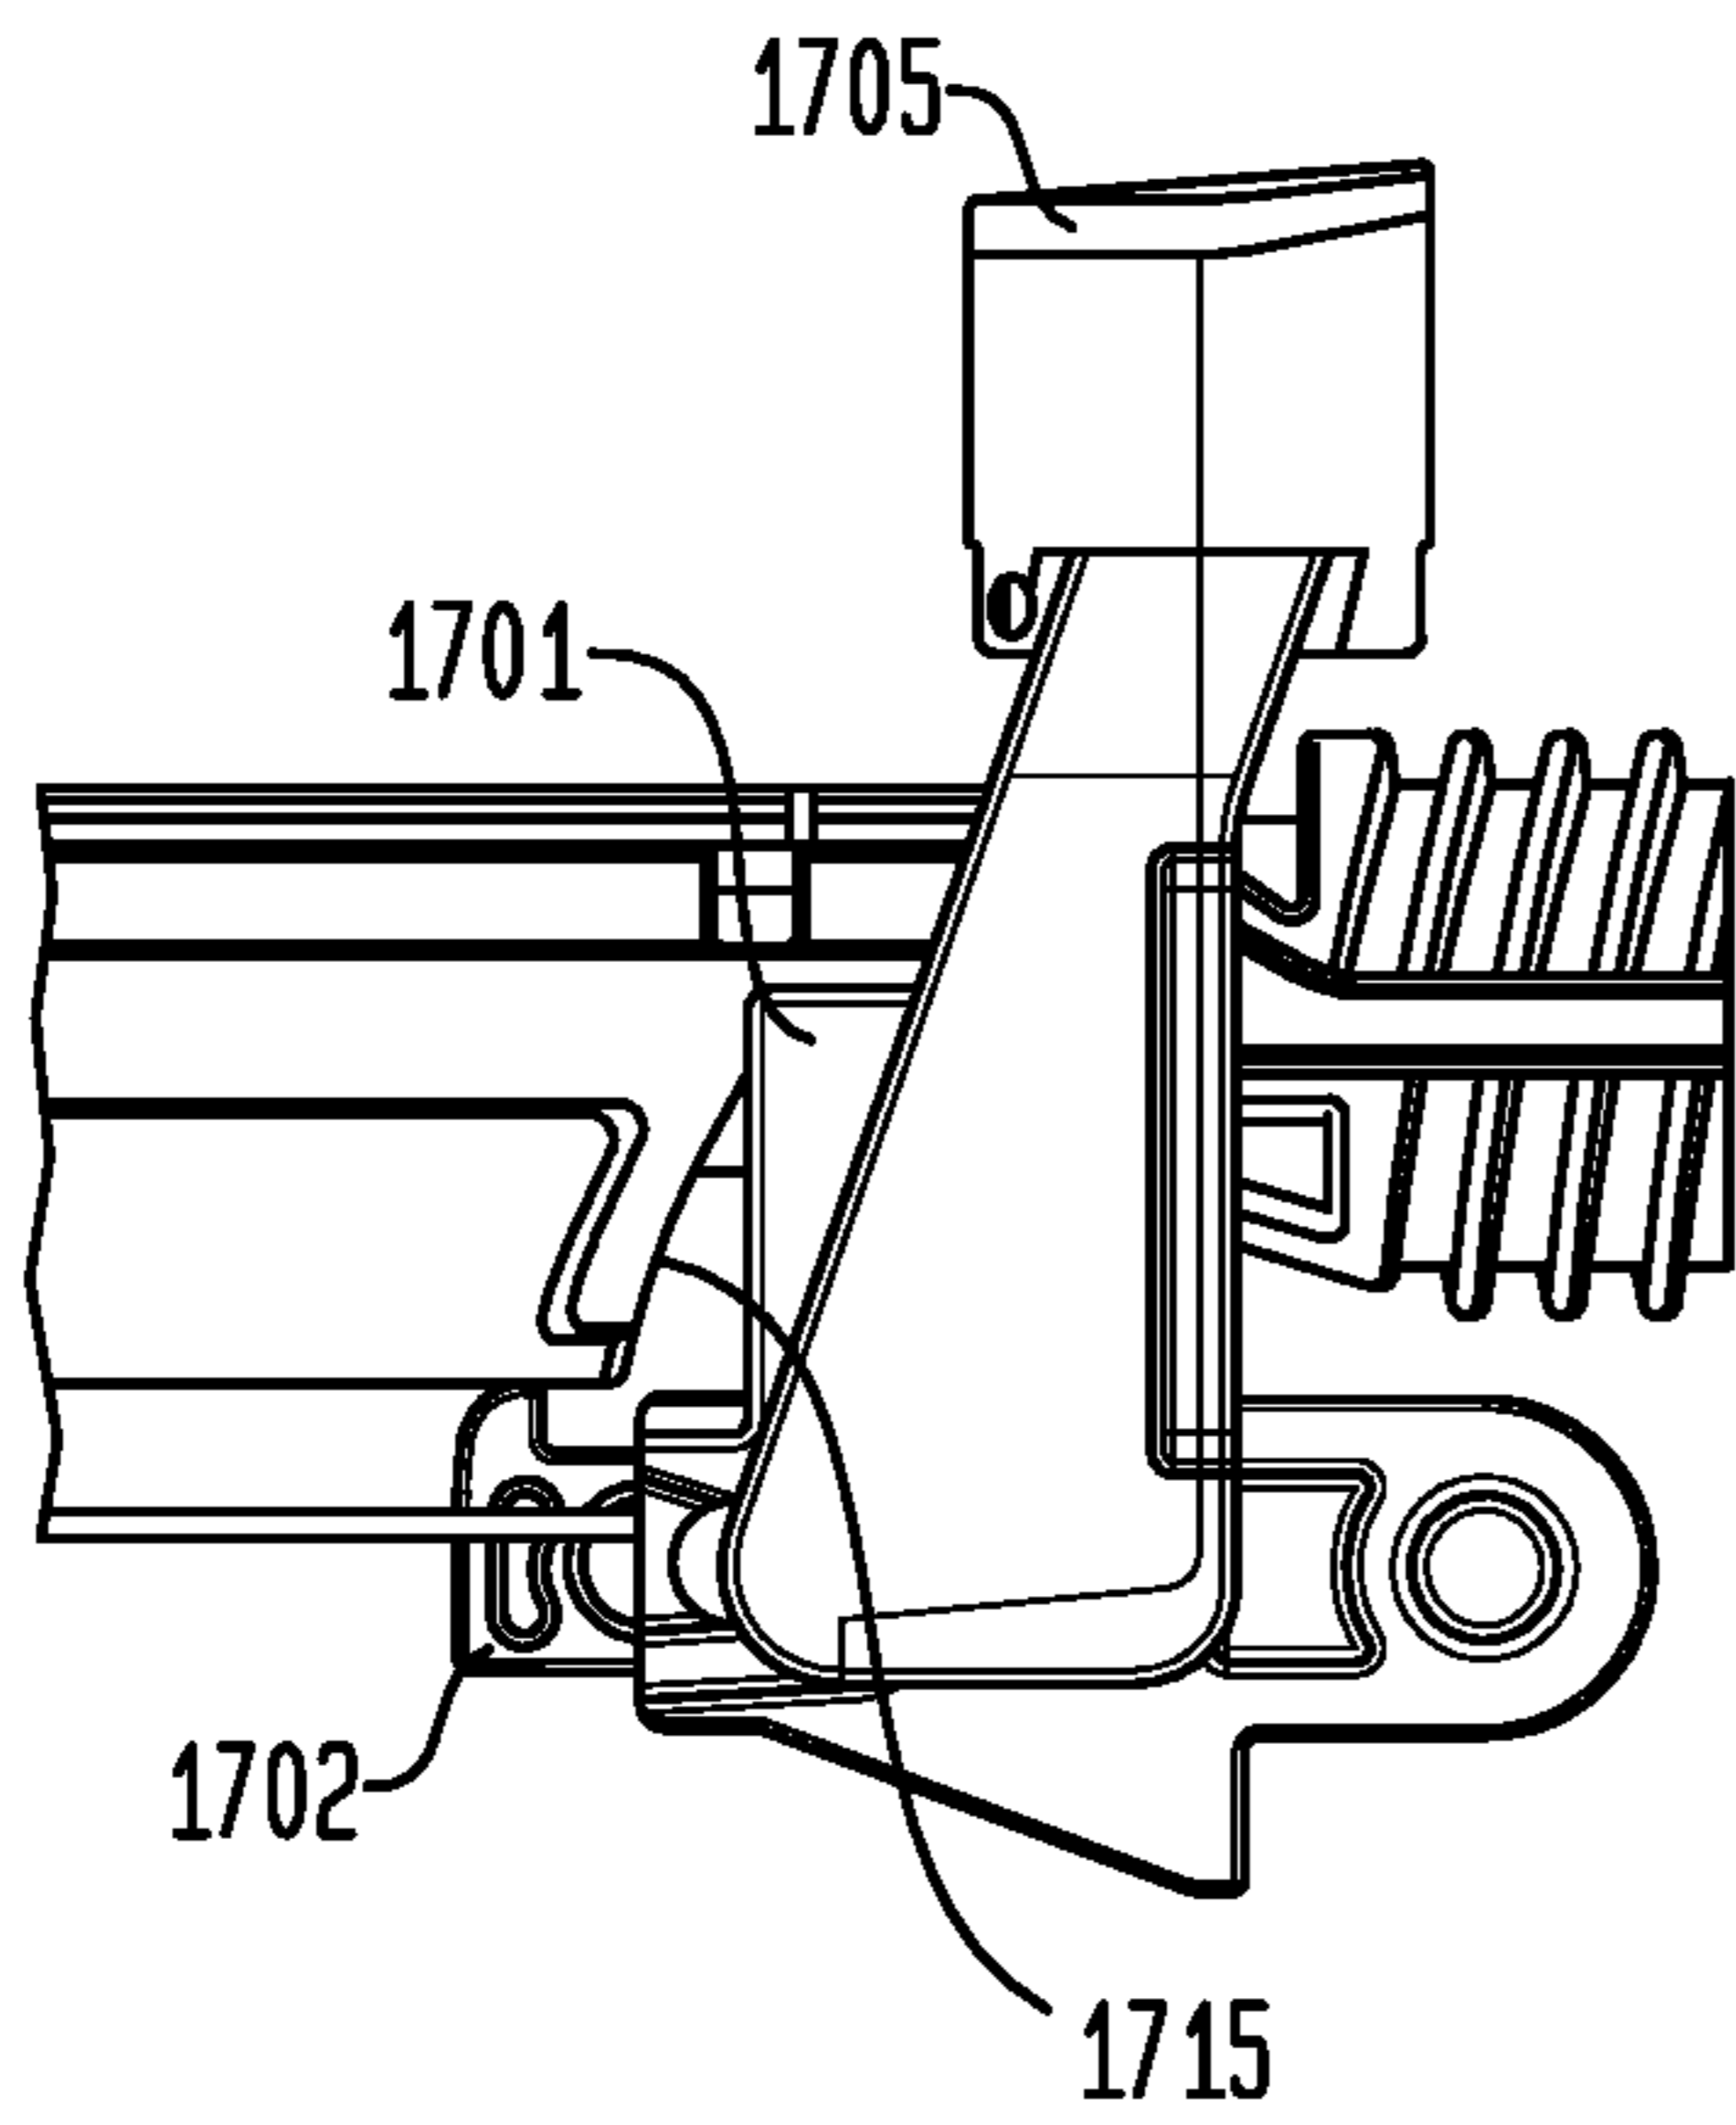




FIG. 10A

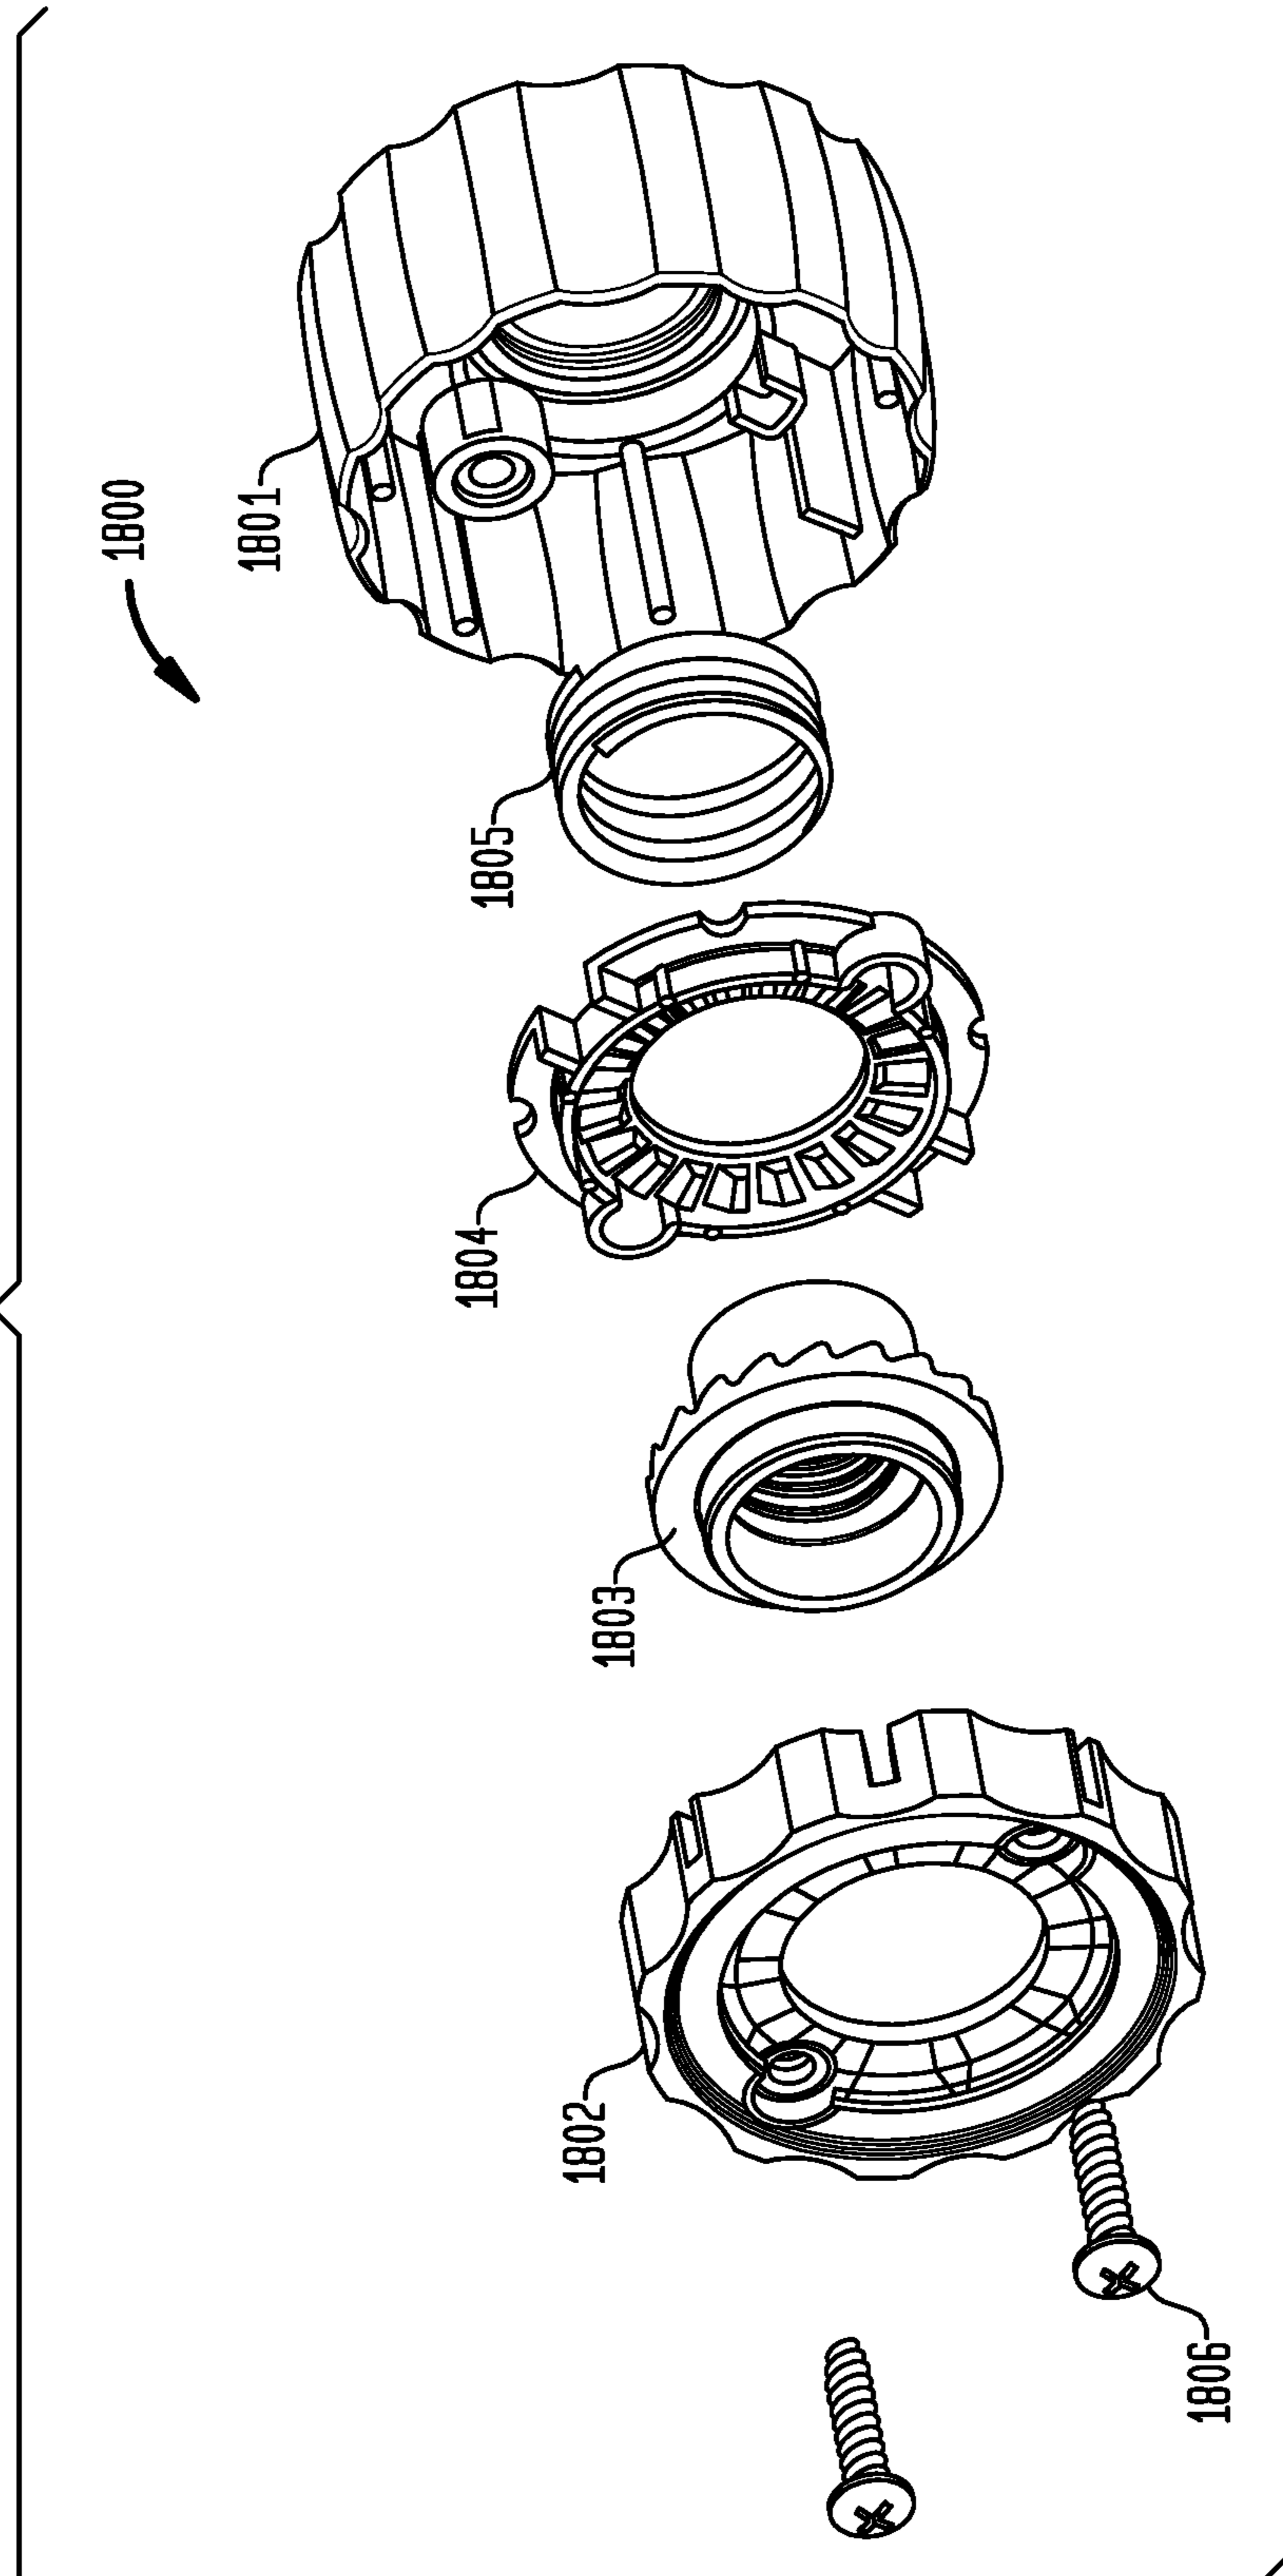


FIG. 10B

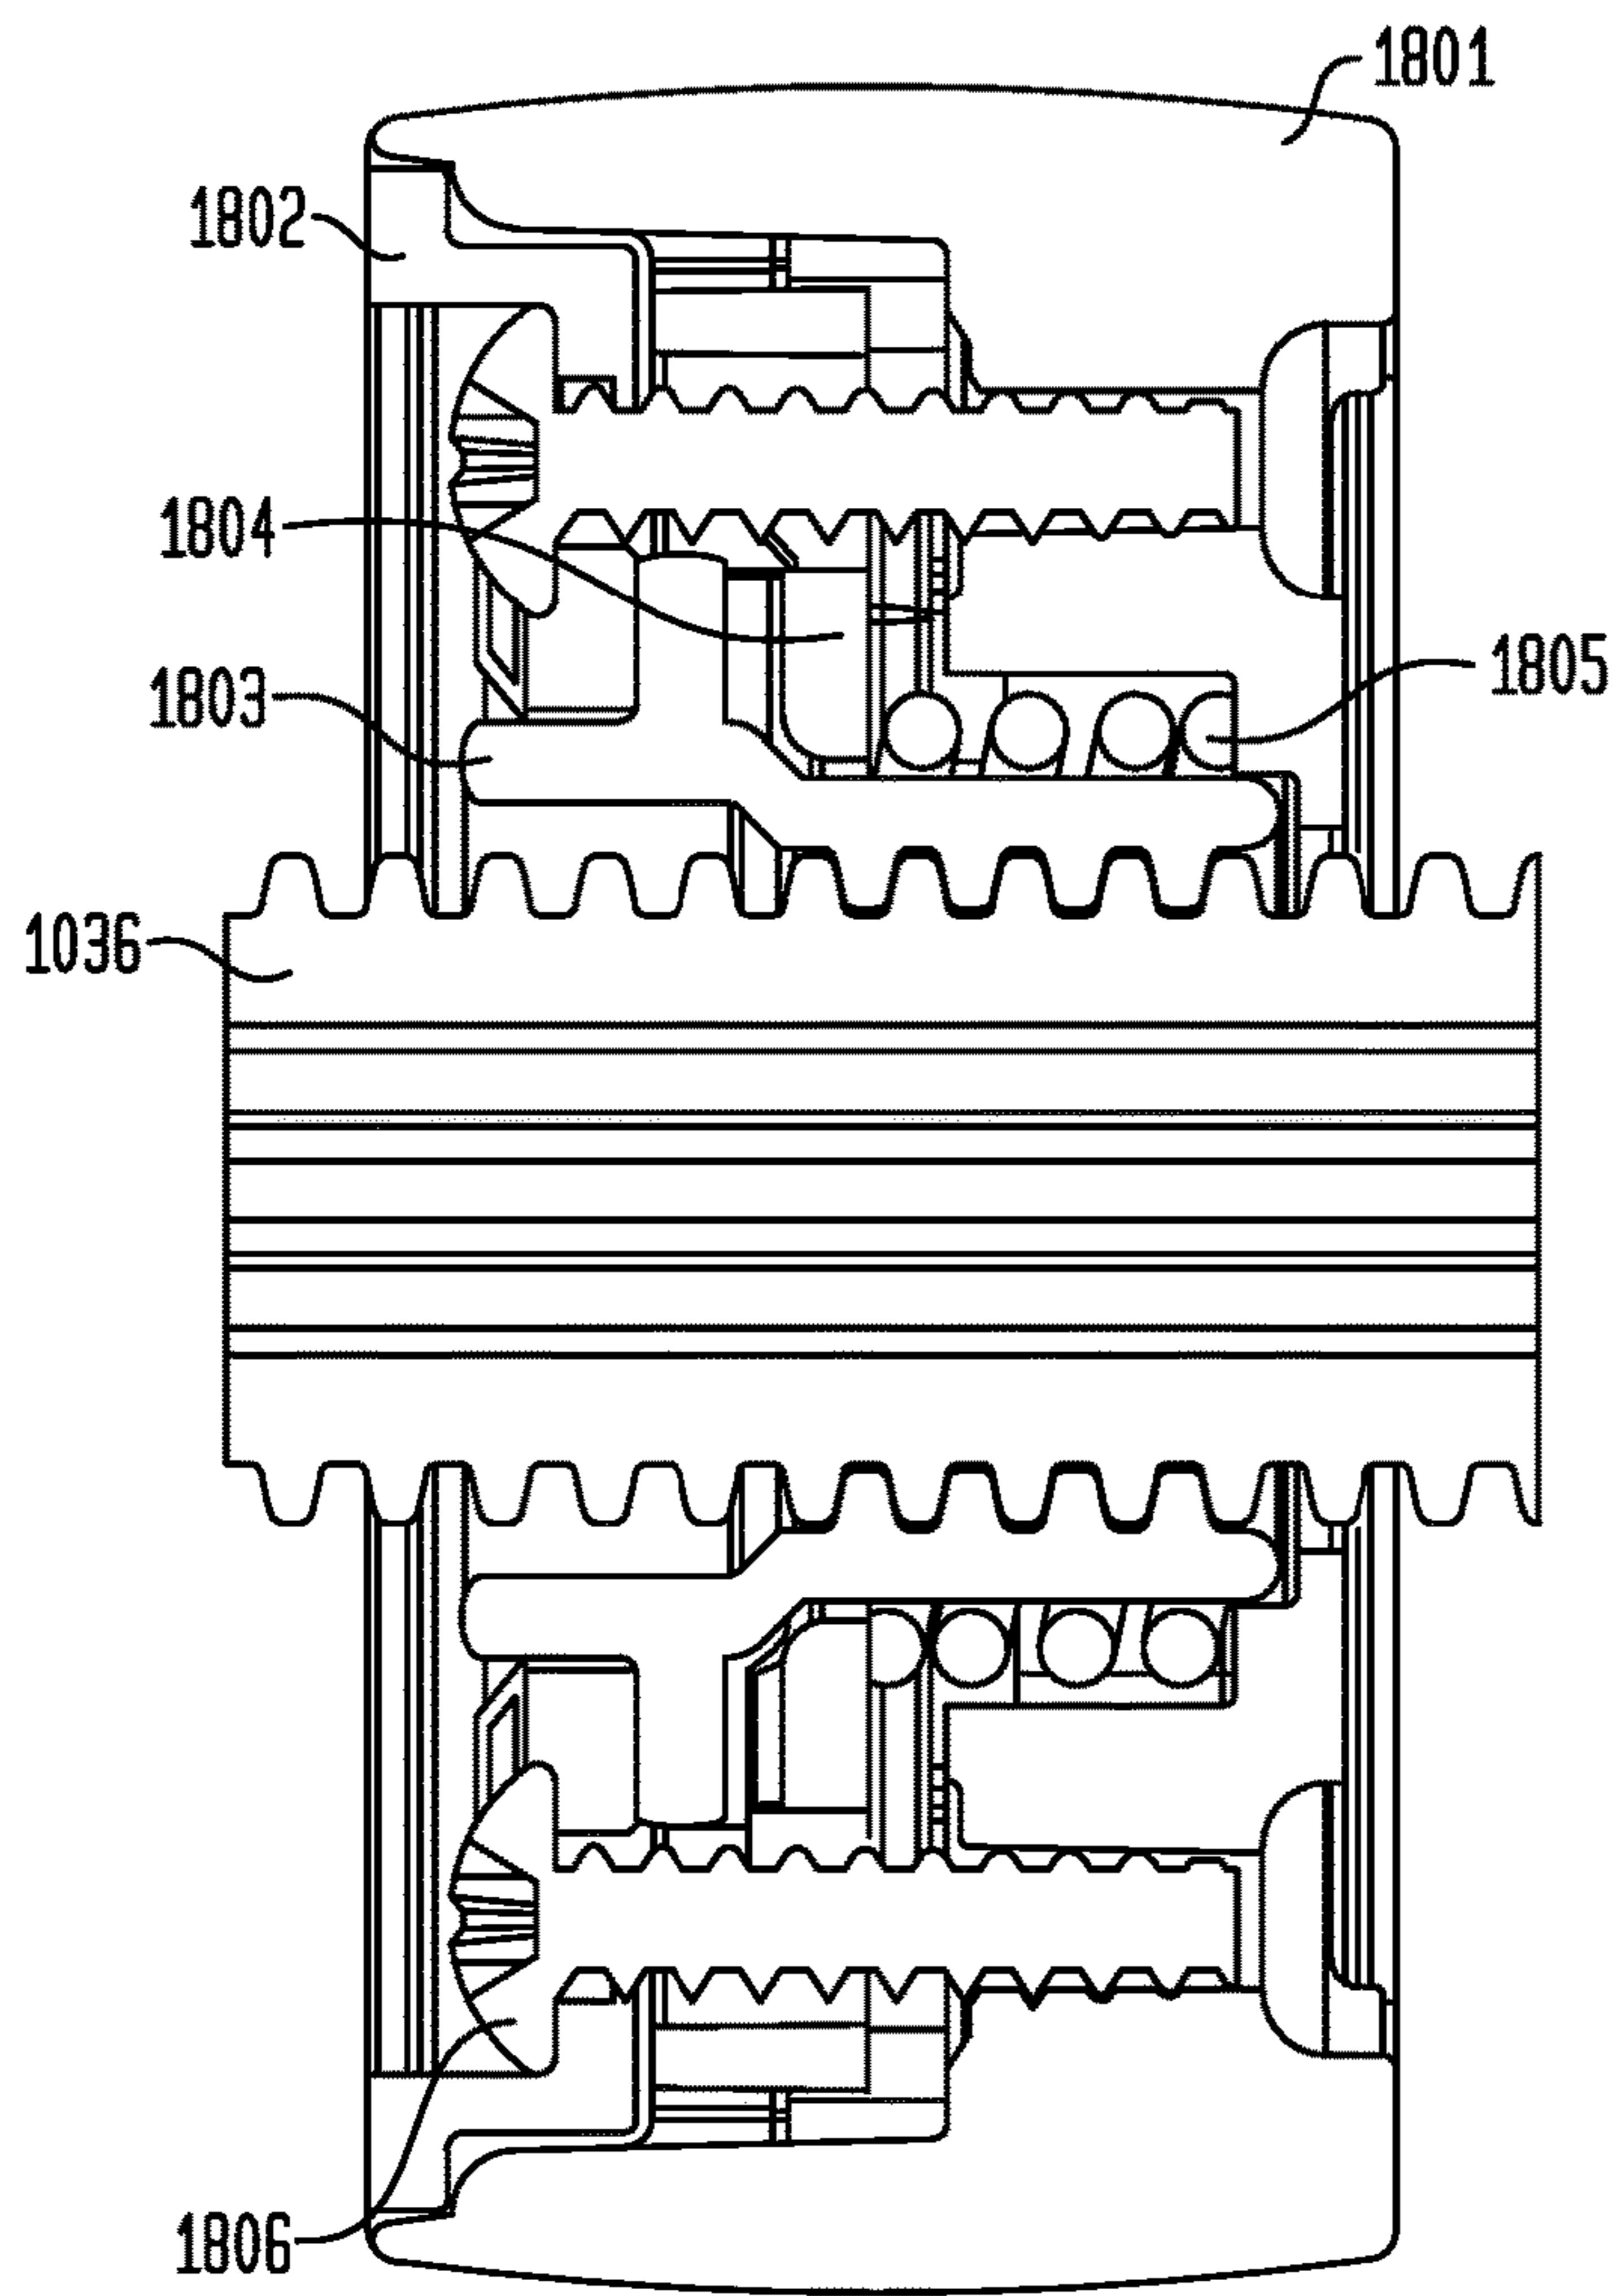


FIG. 10C



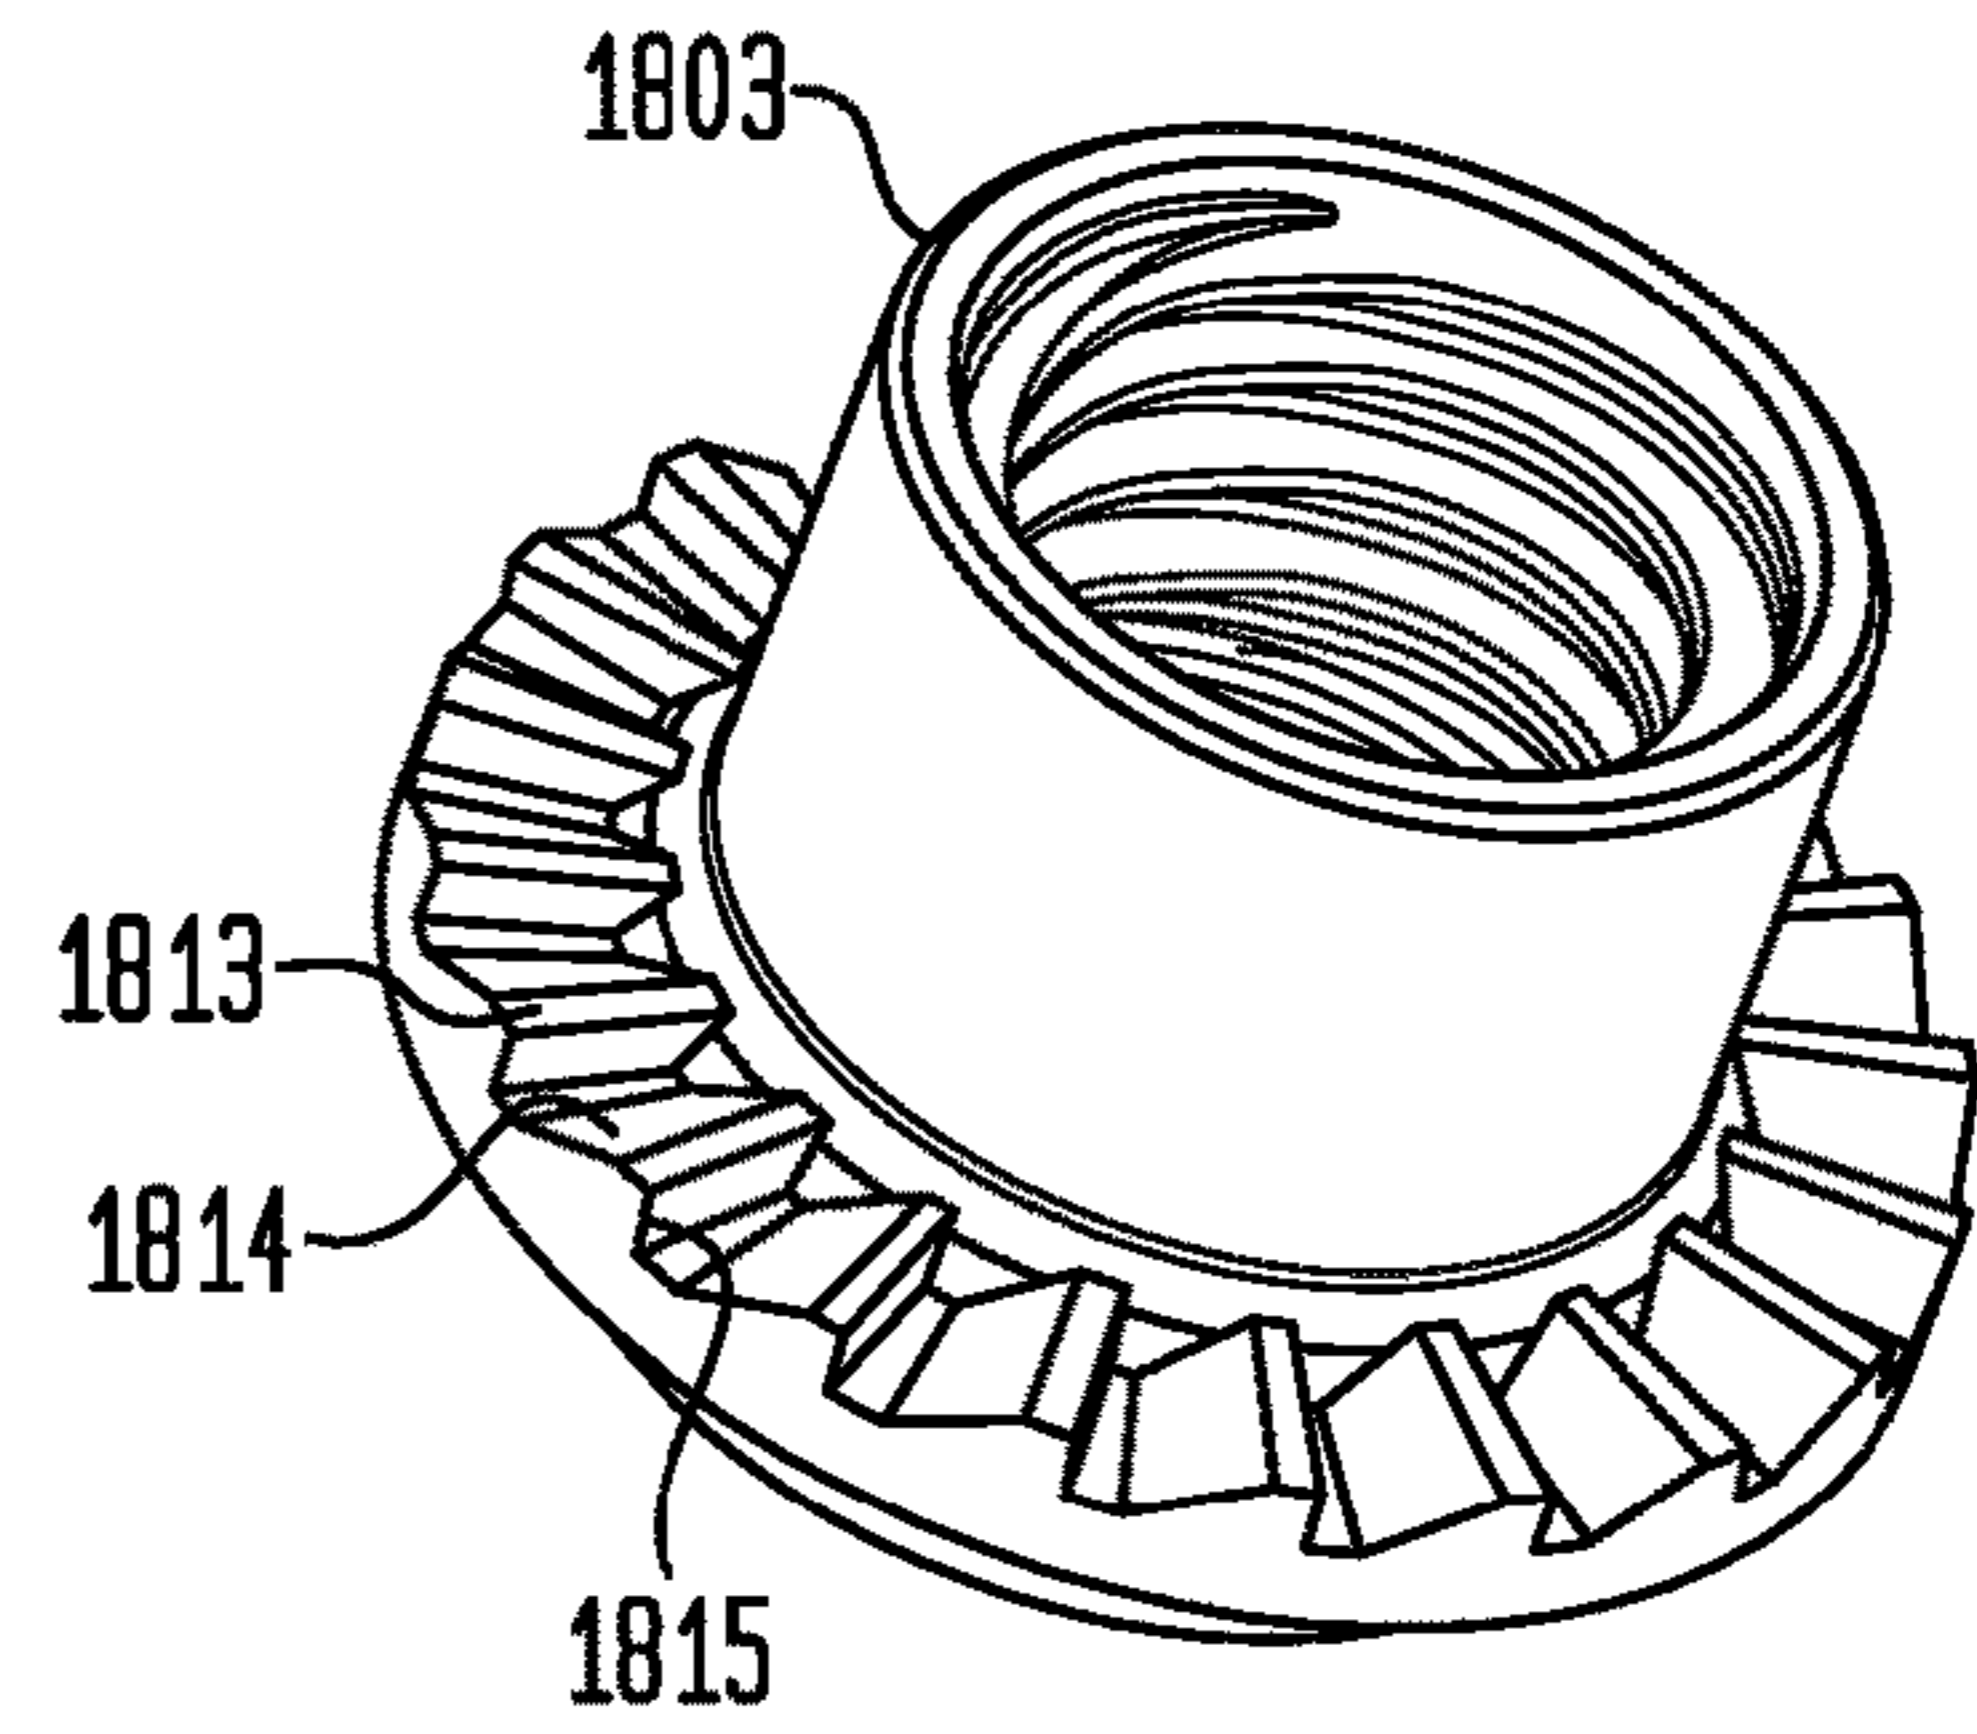


FIG. 10D

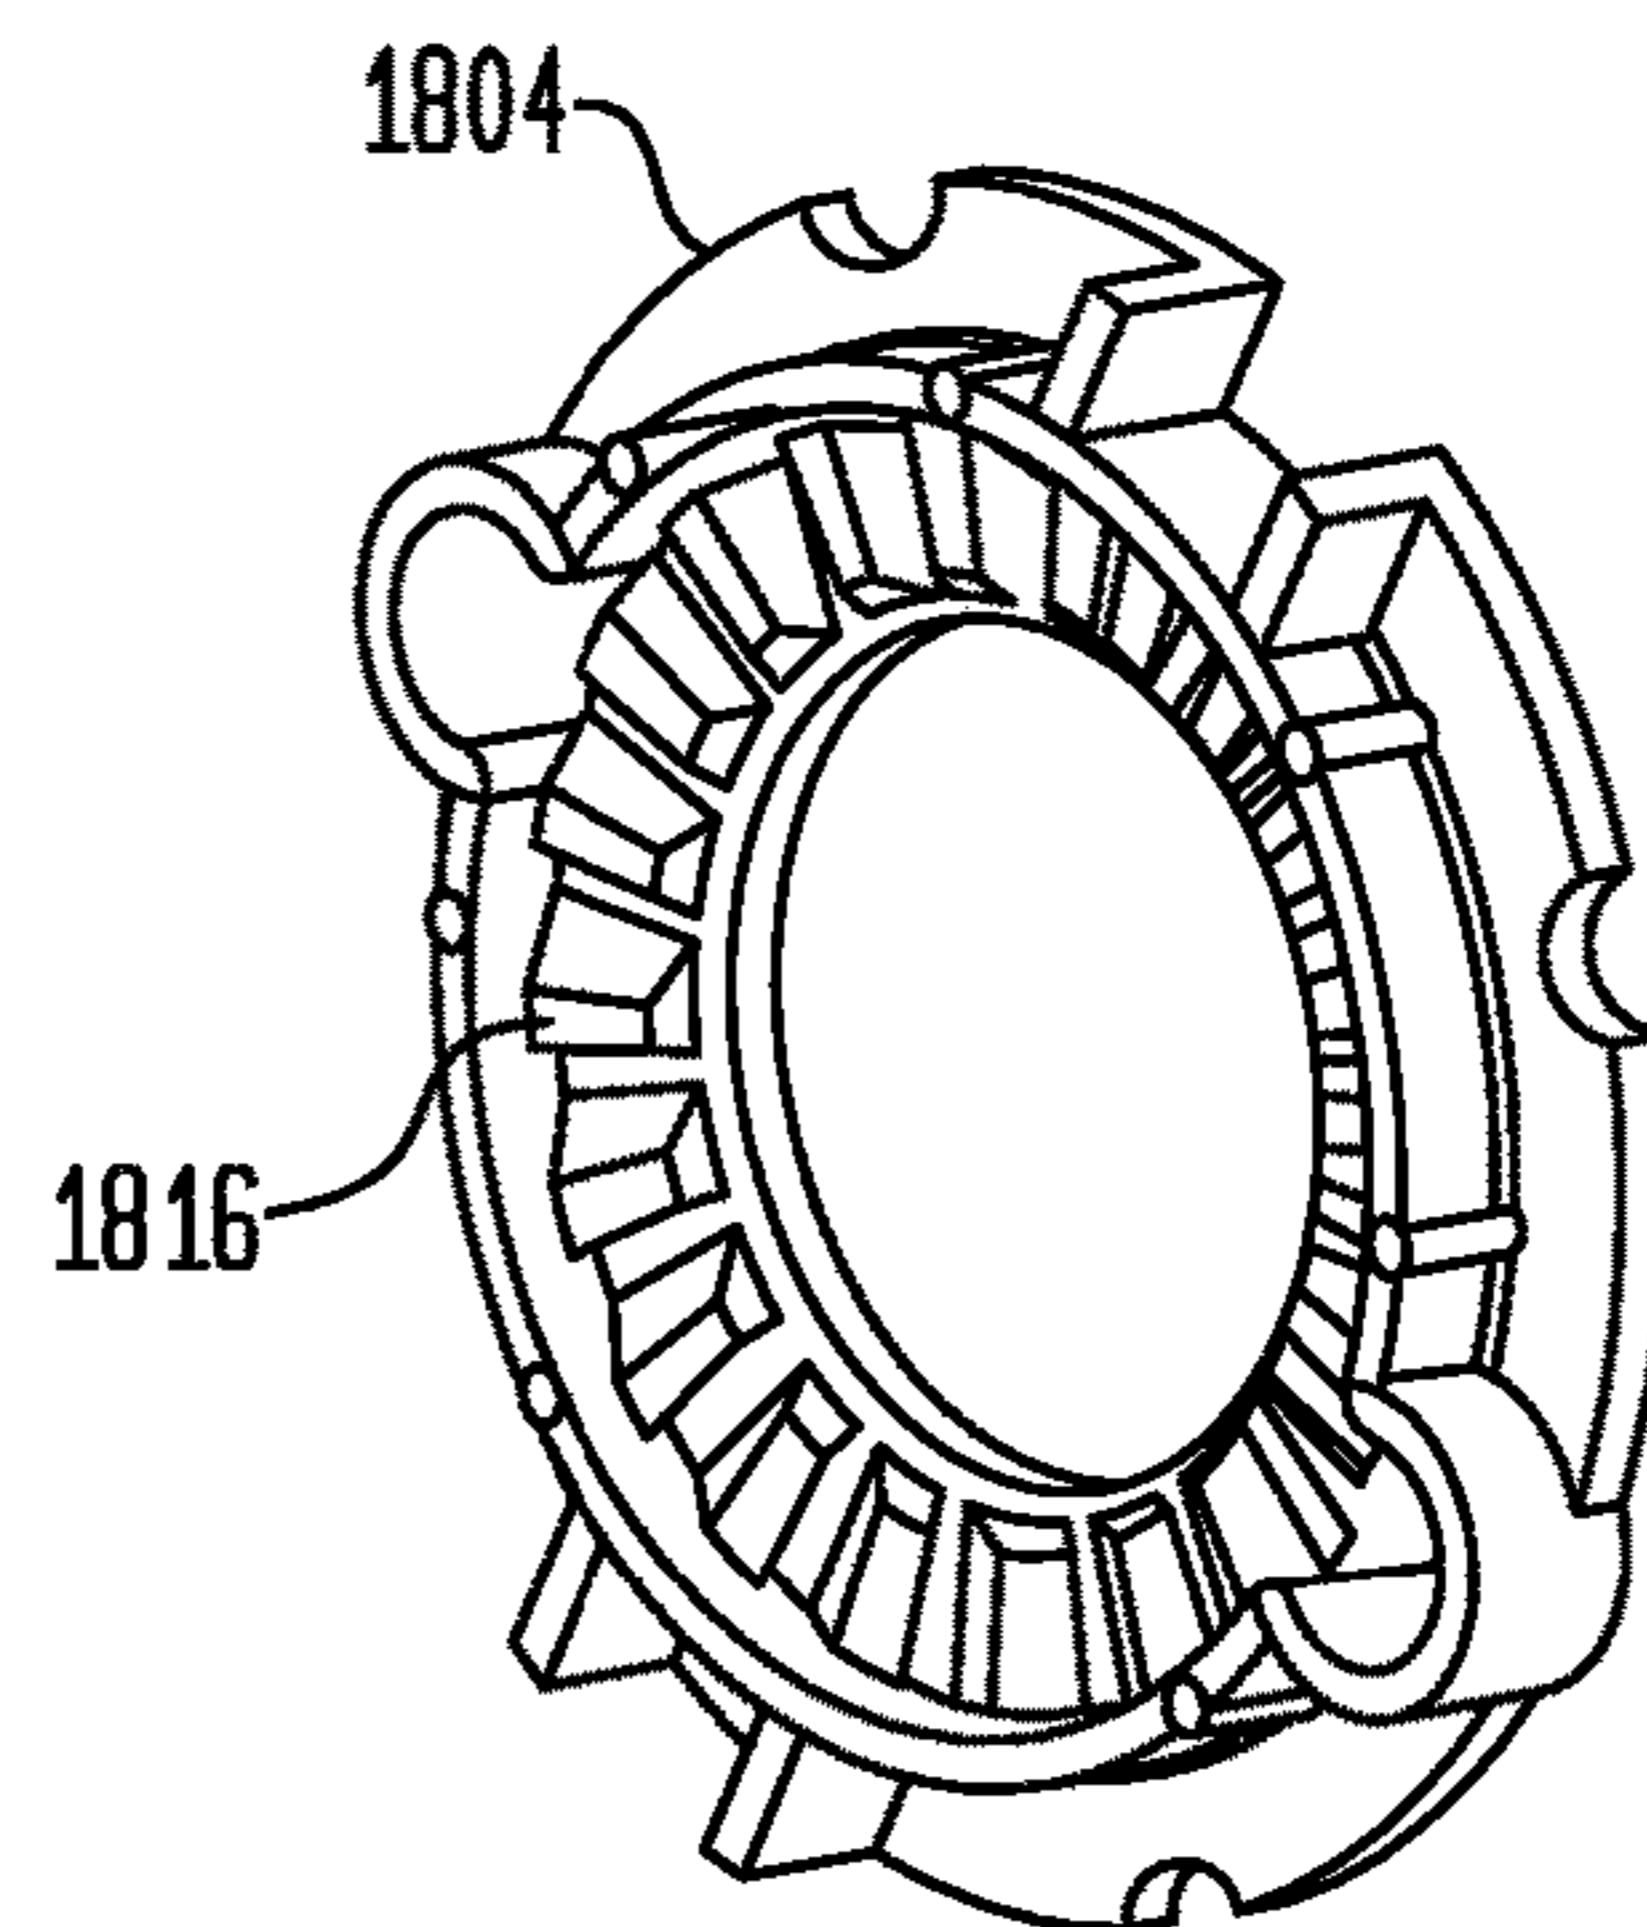

**FIG. 11A**

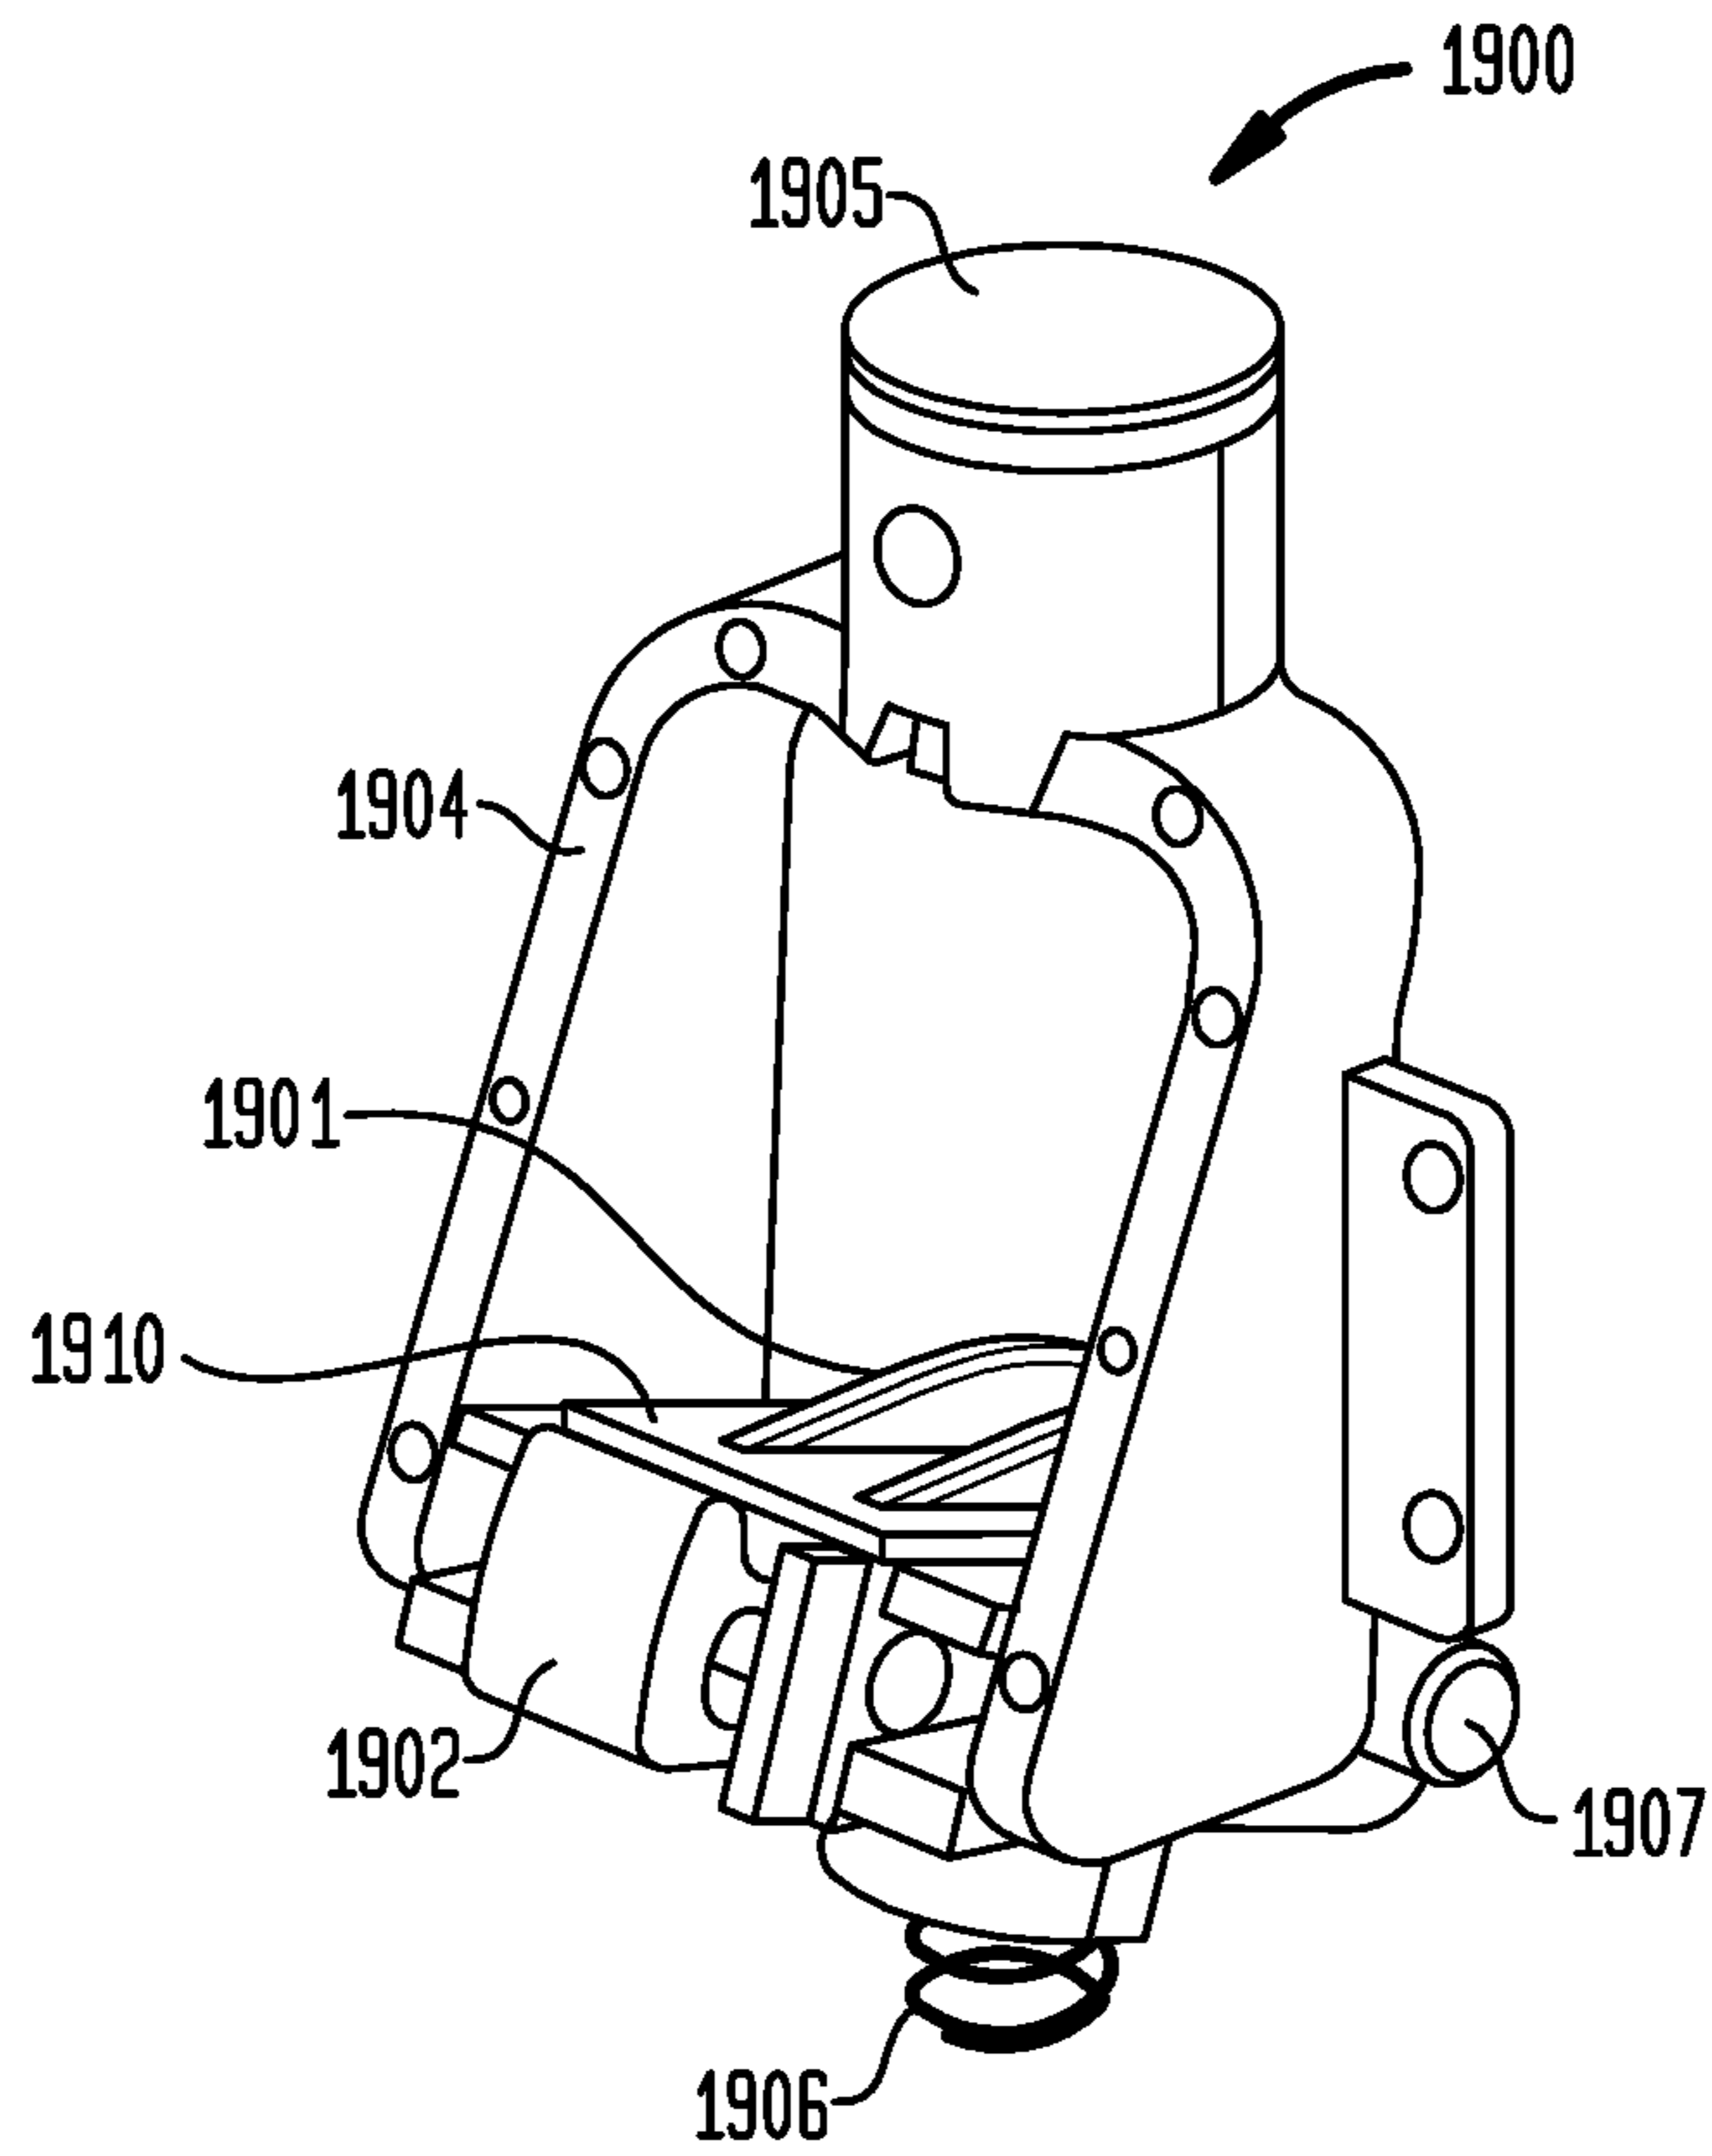

**FIG. 11B**

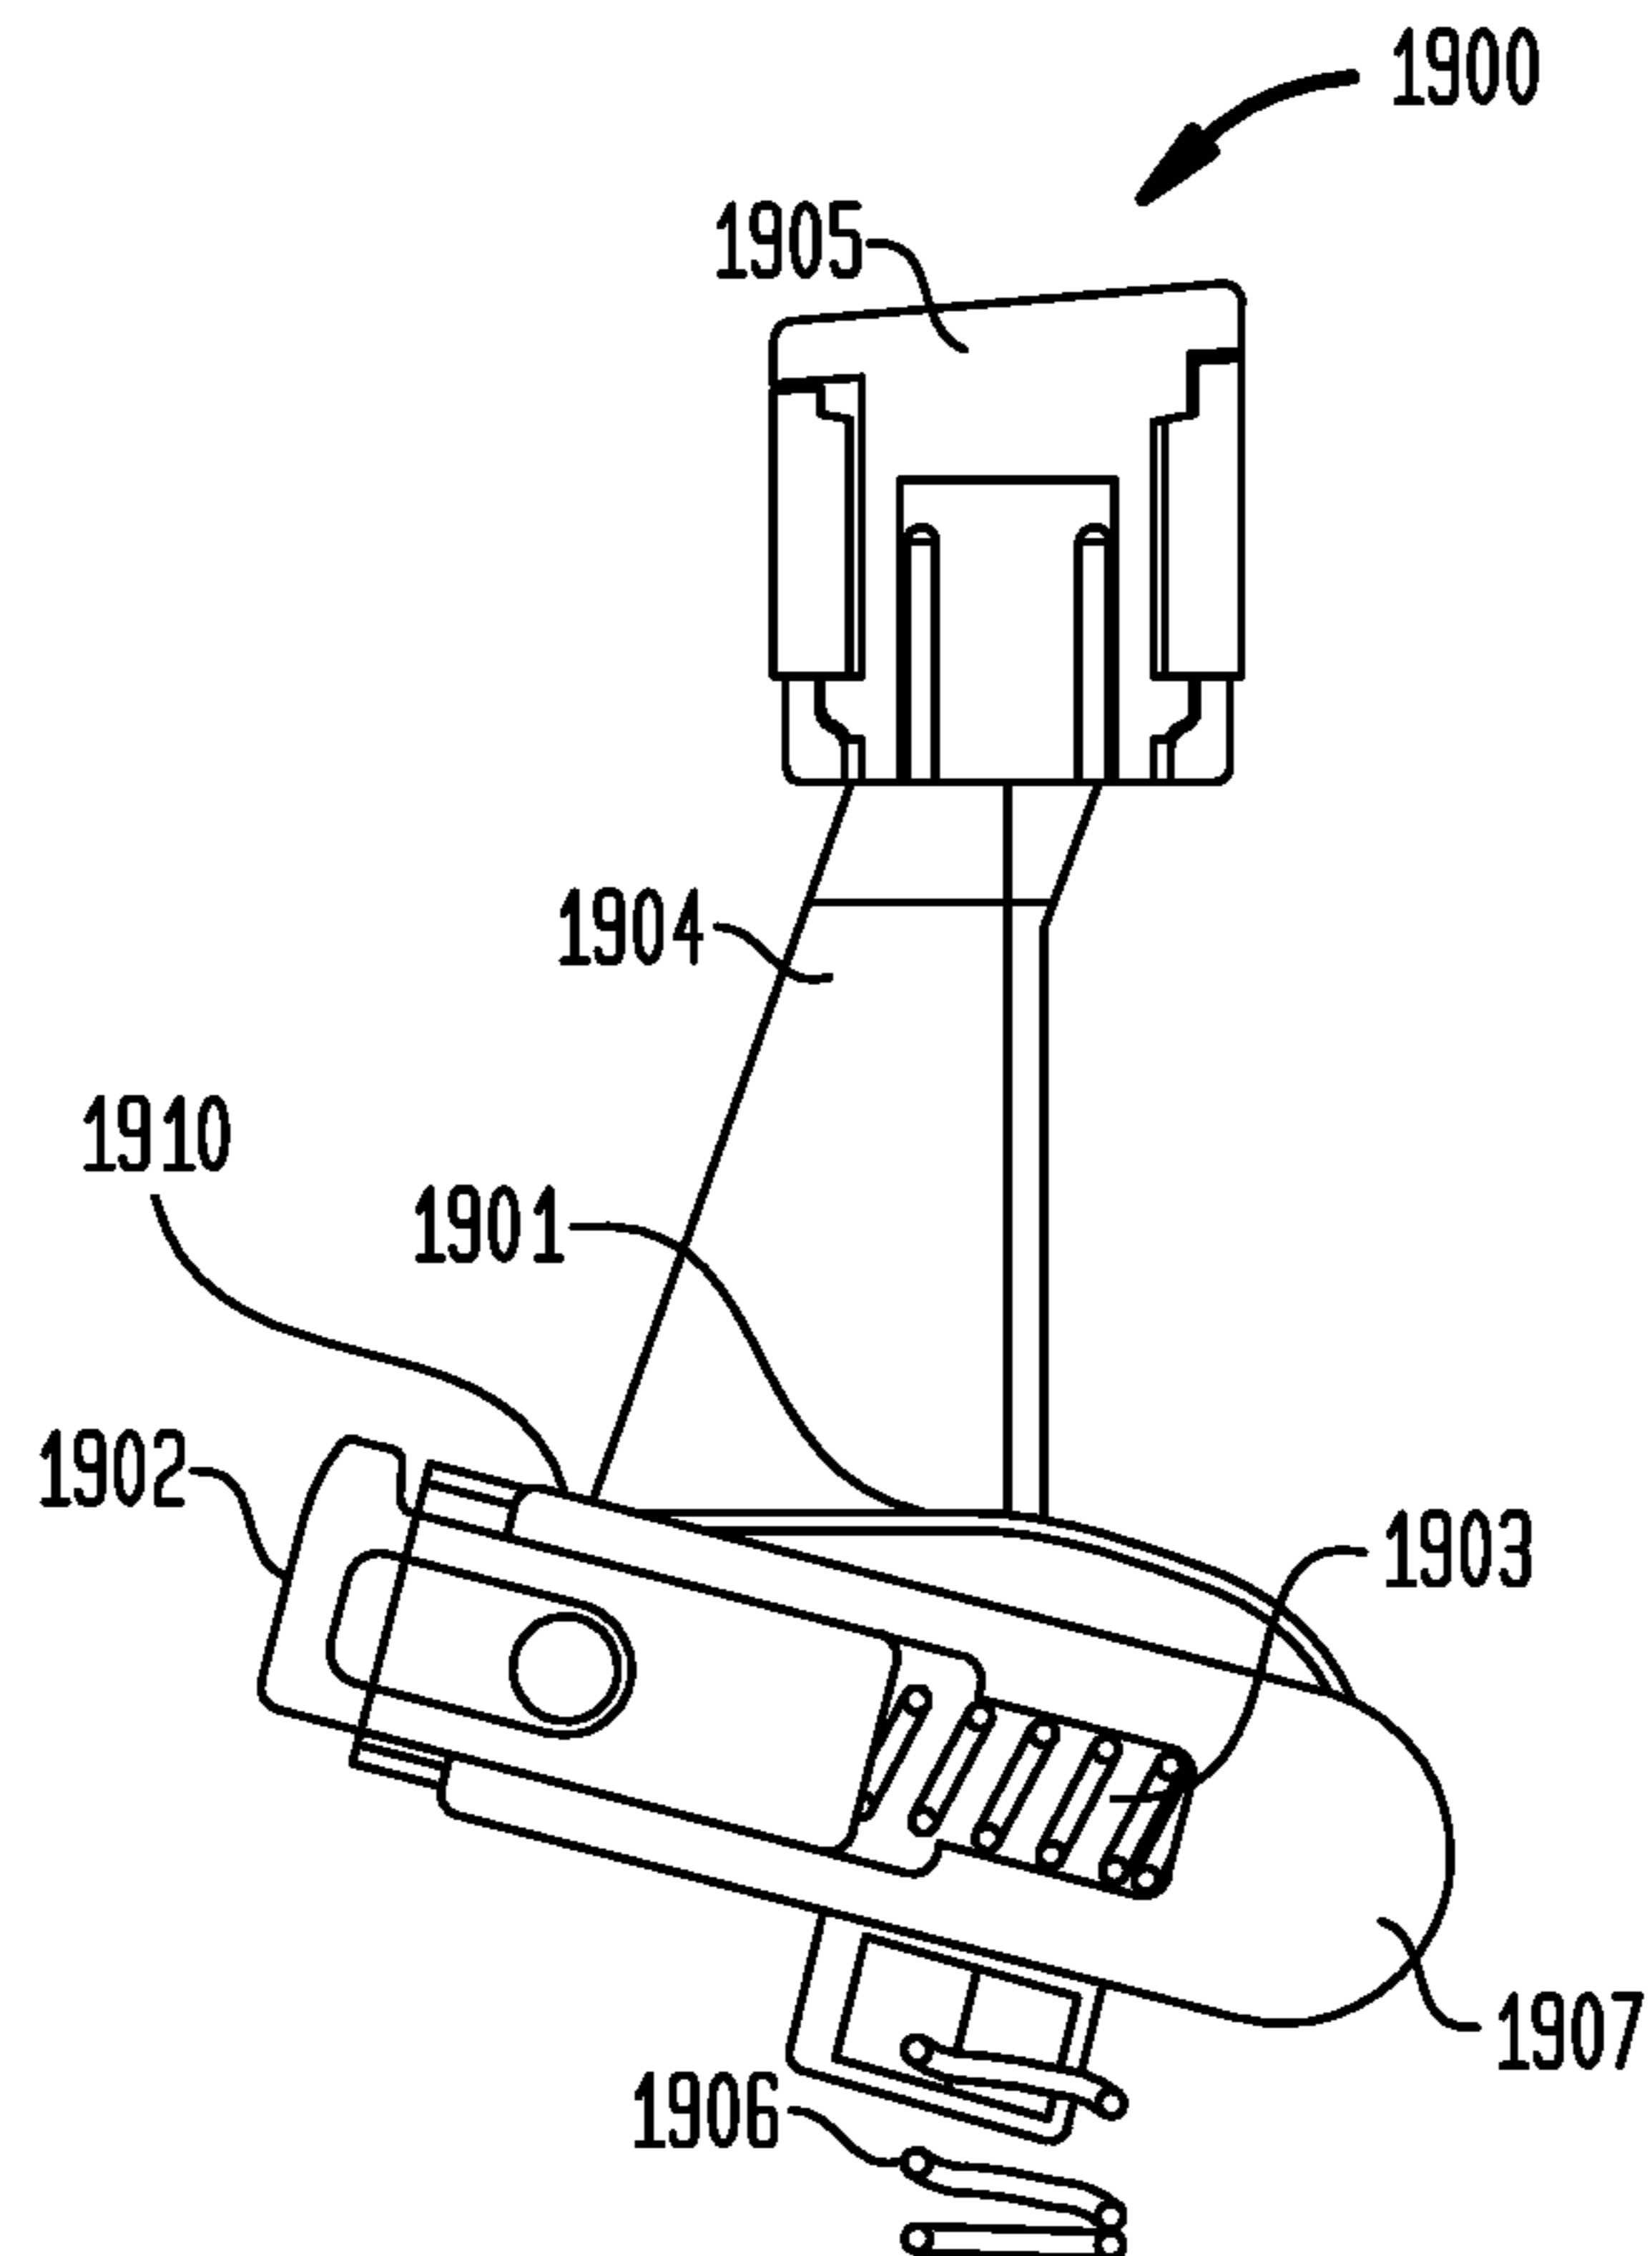


FIG. 11C

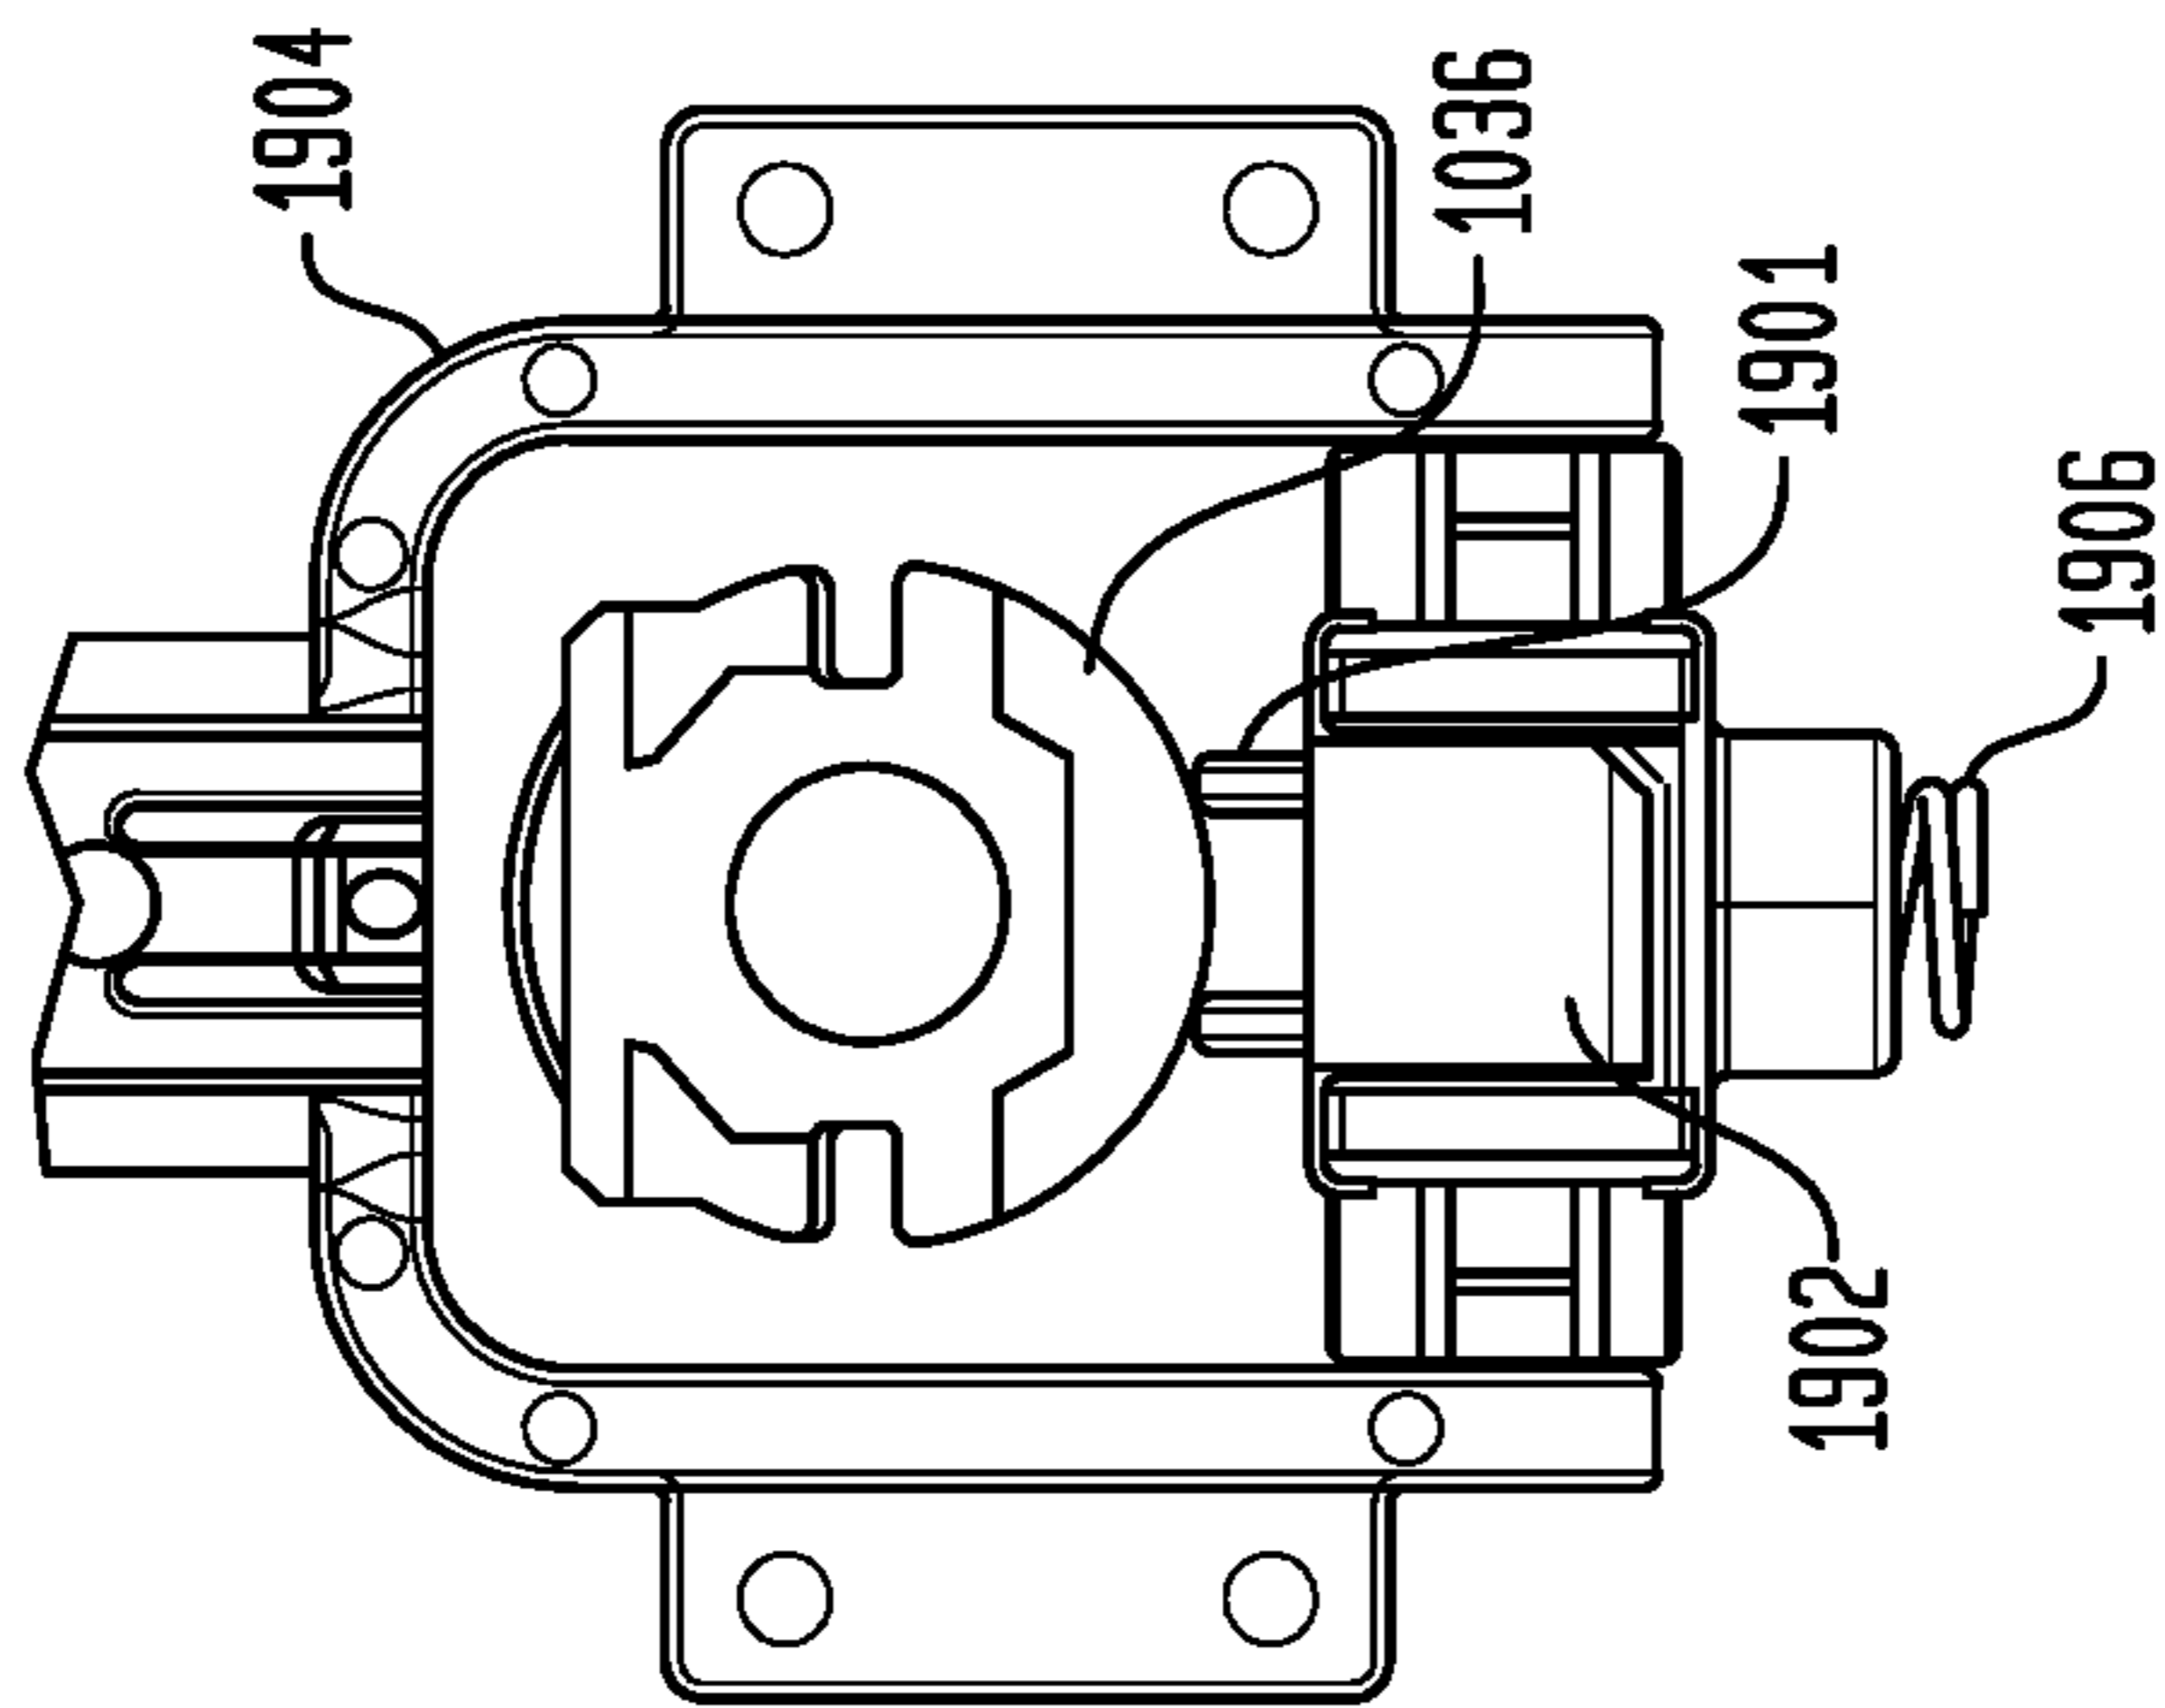


FIG. 11D


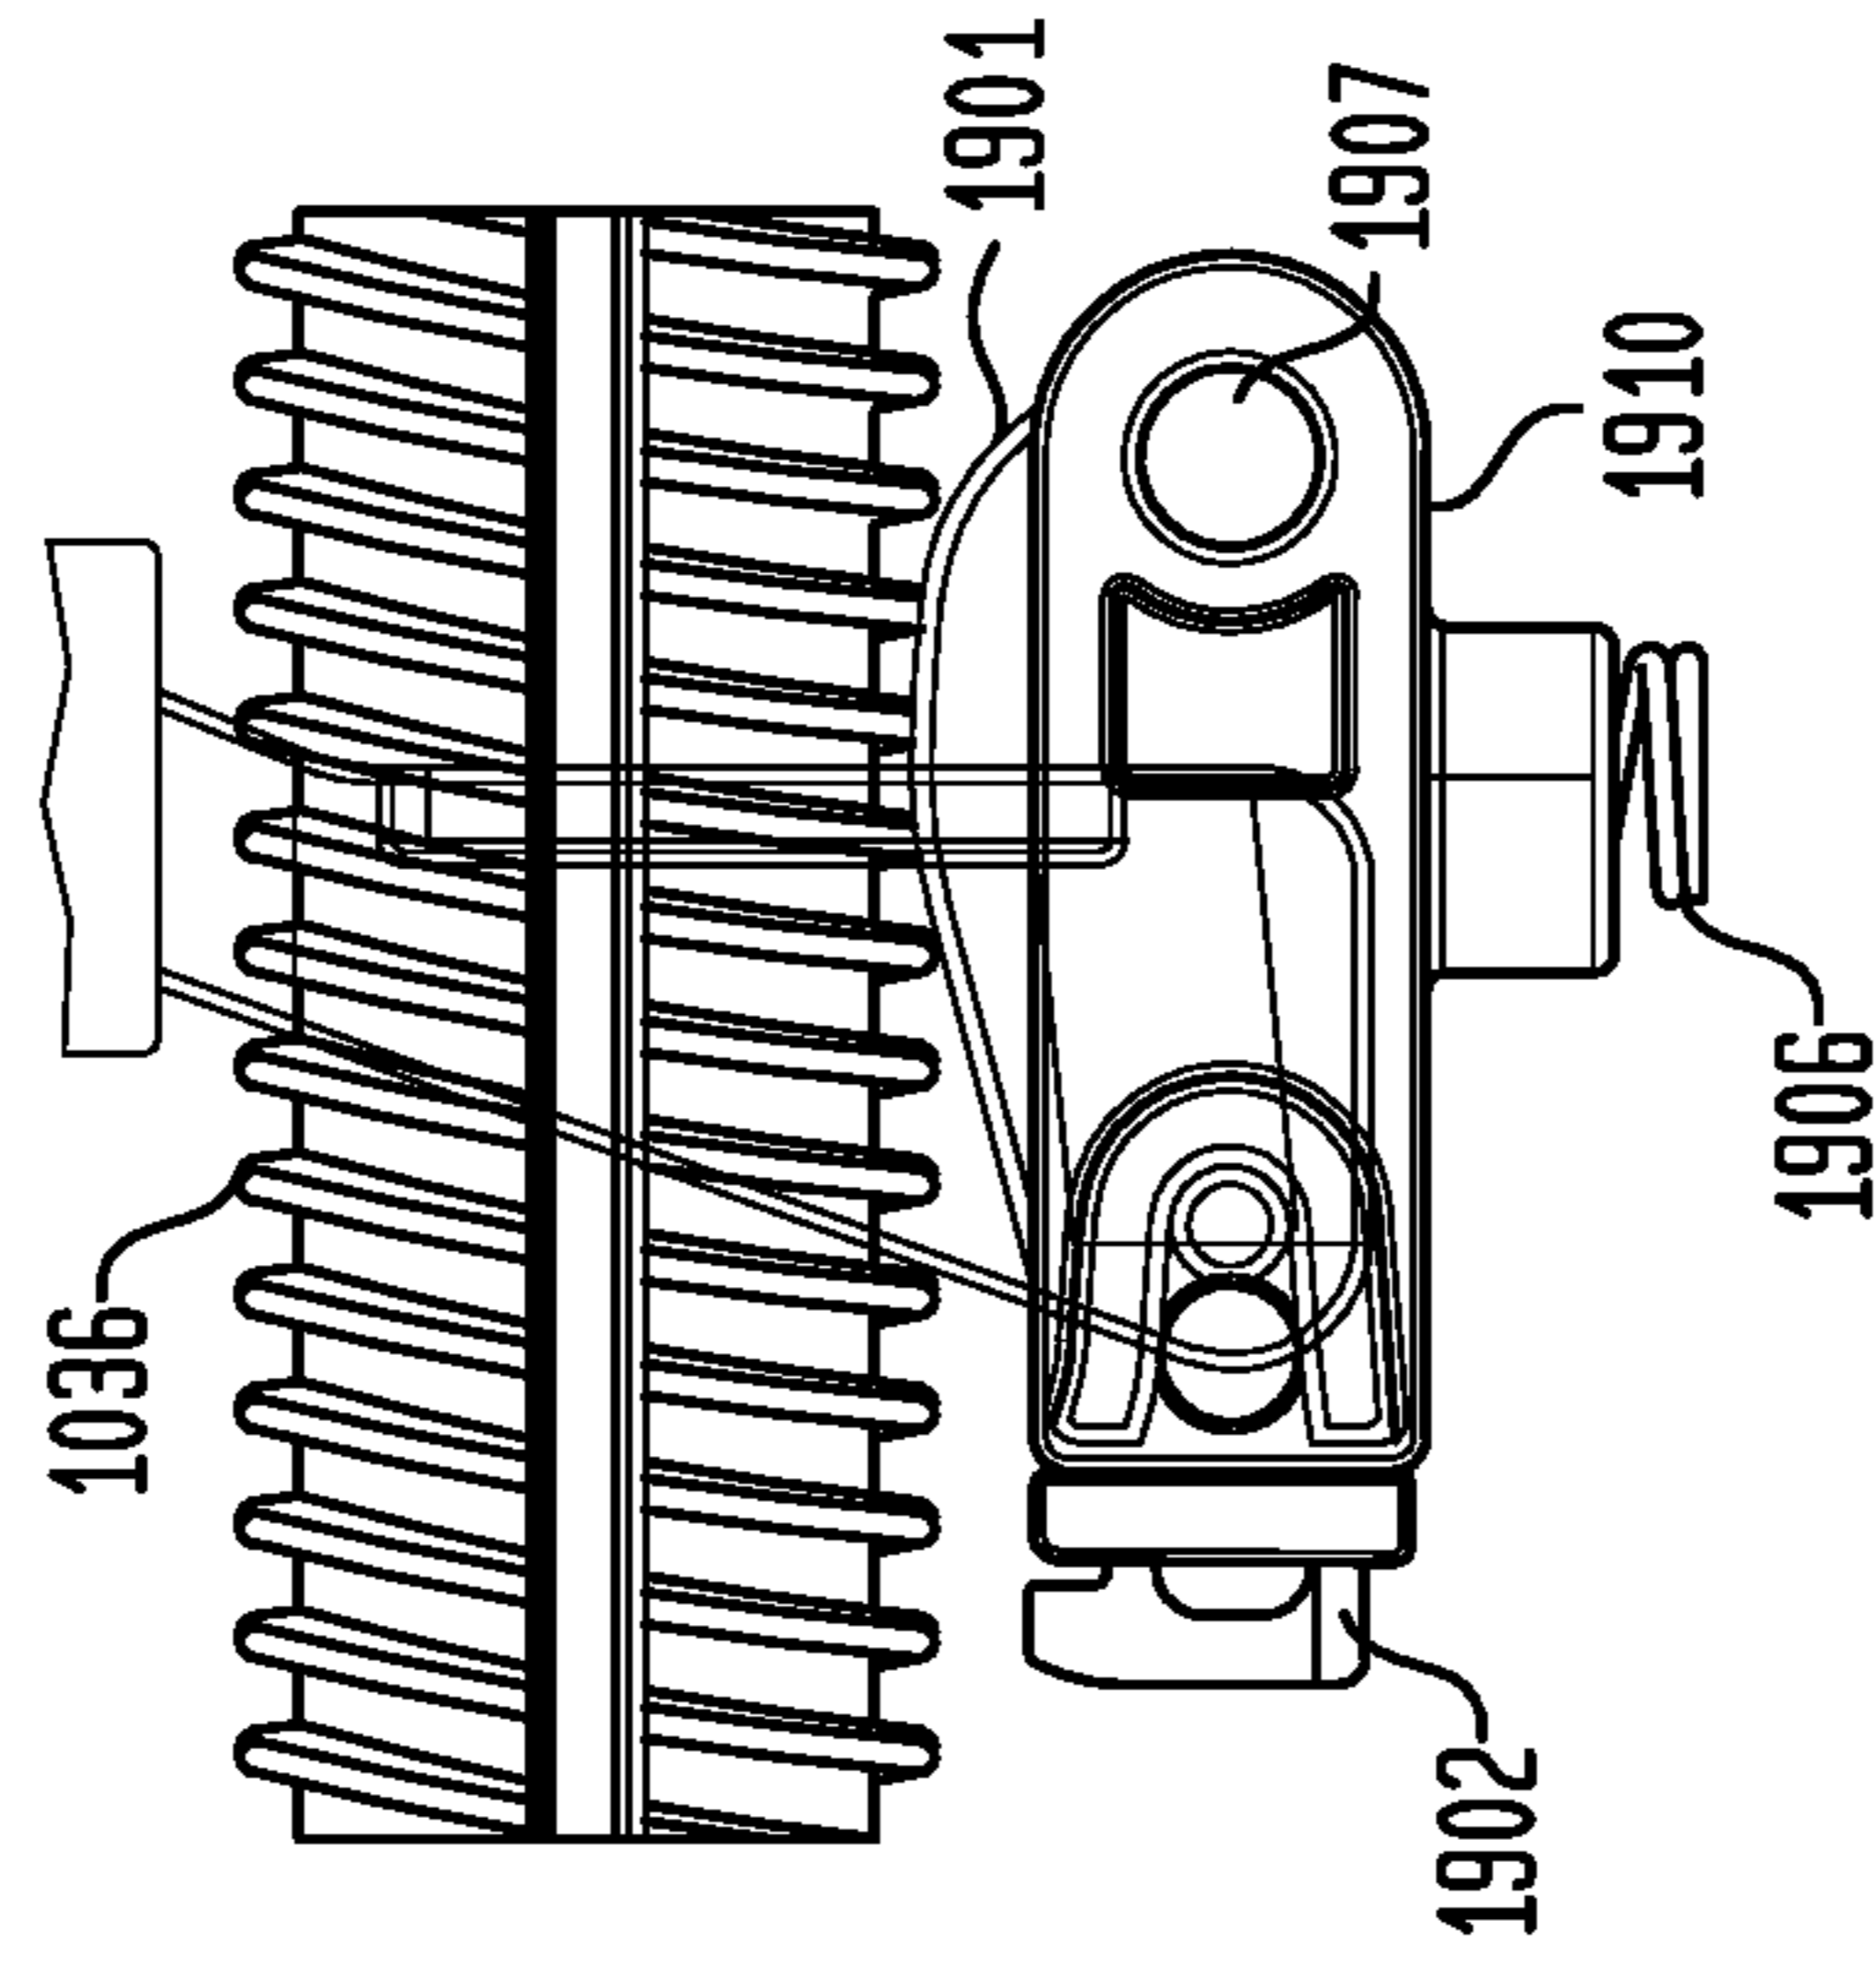


FIG. 11E

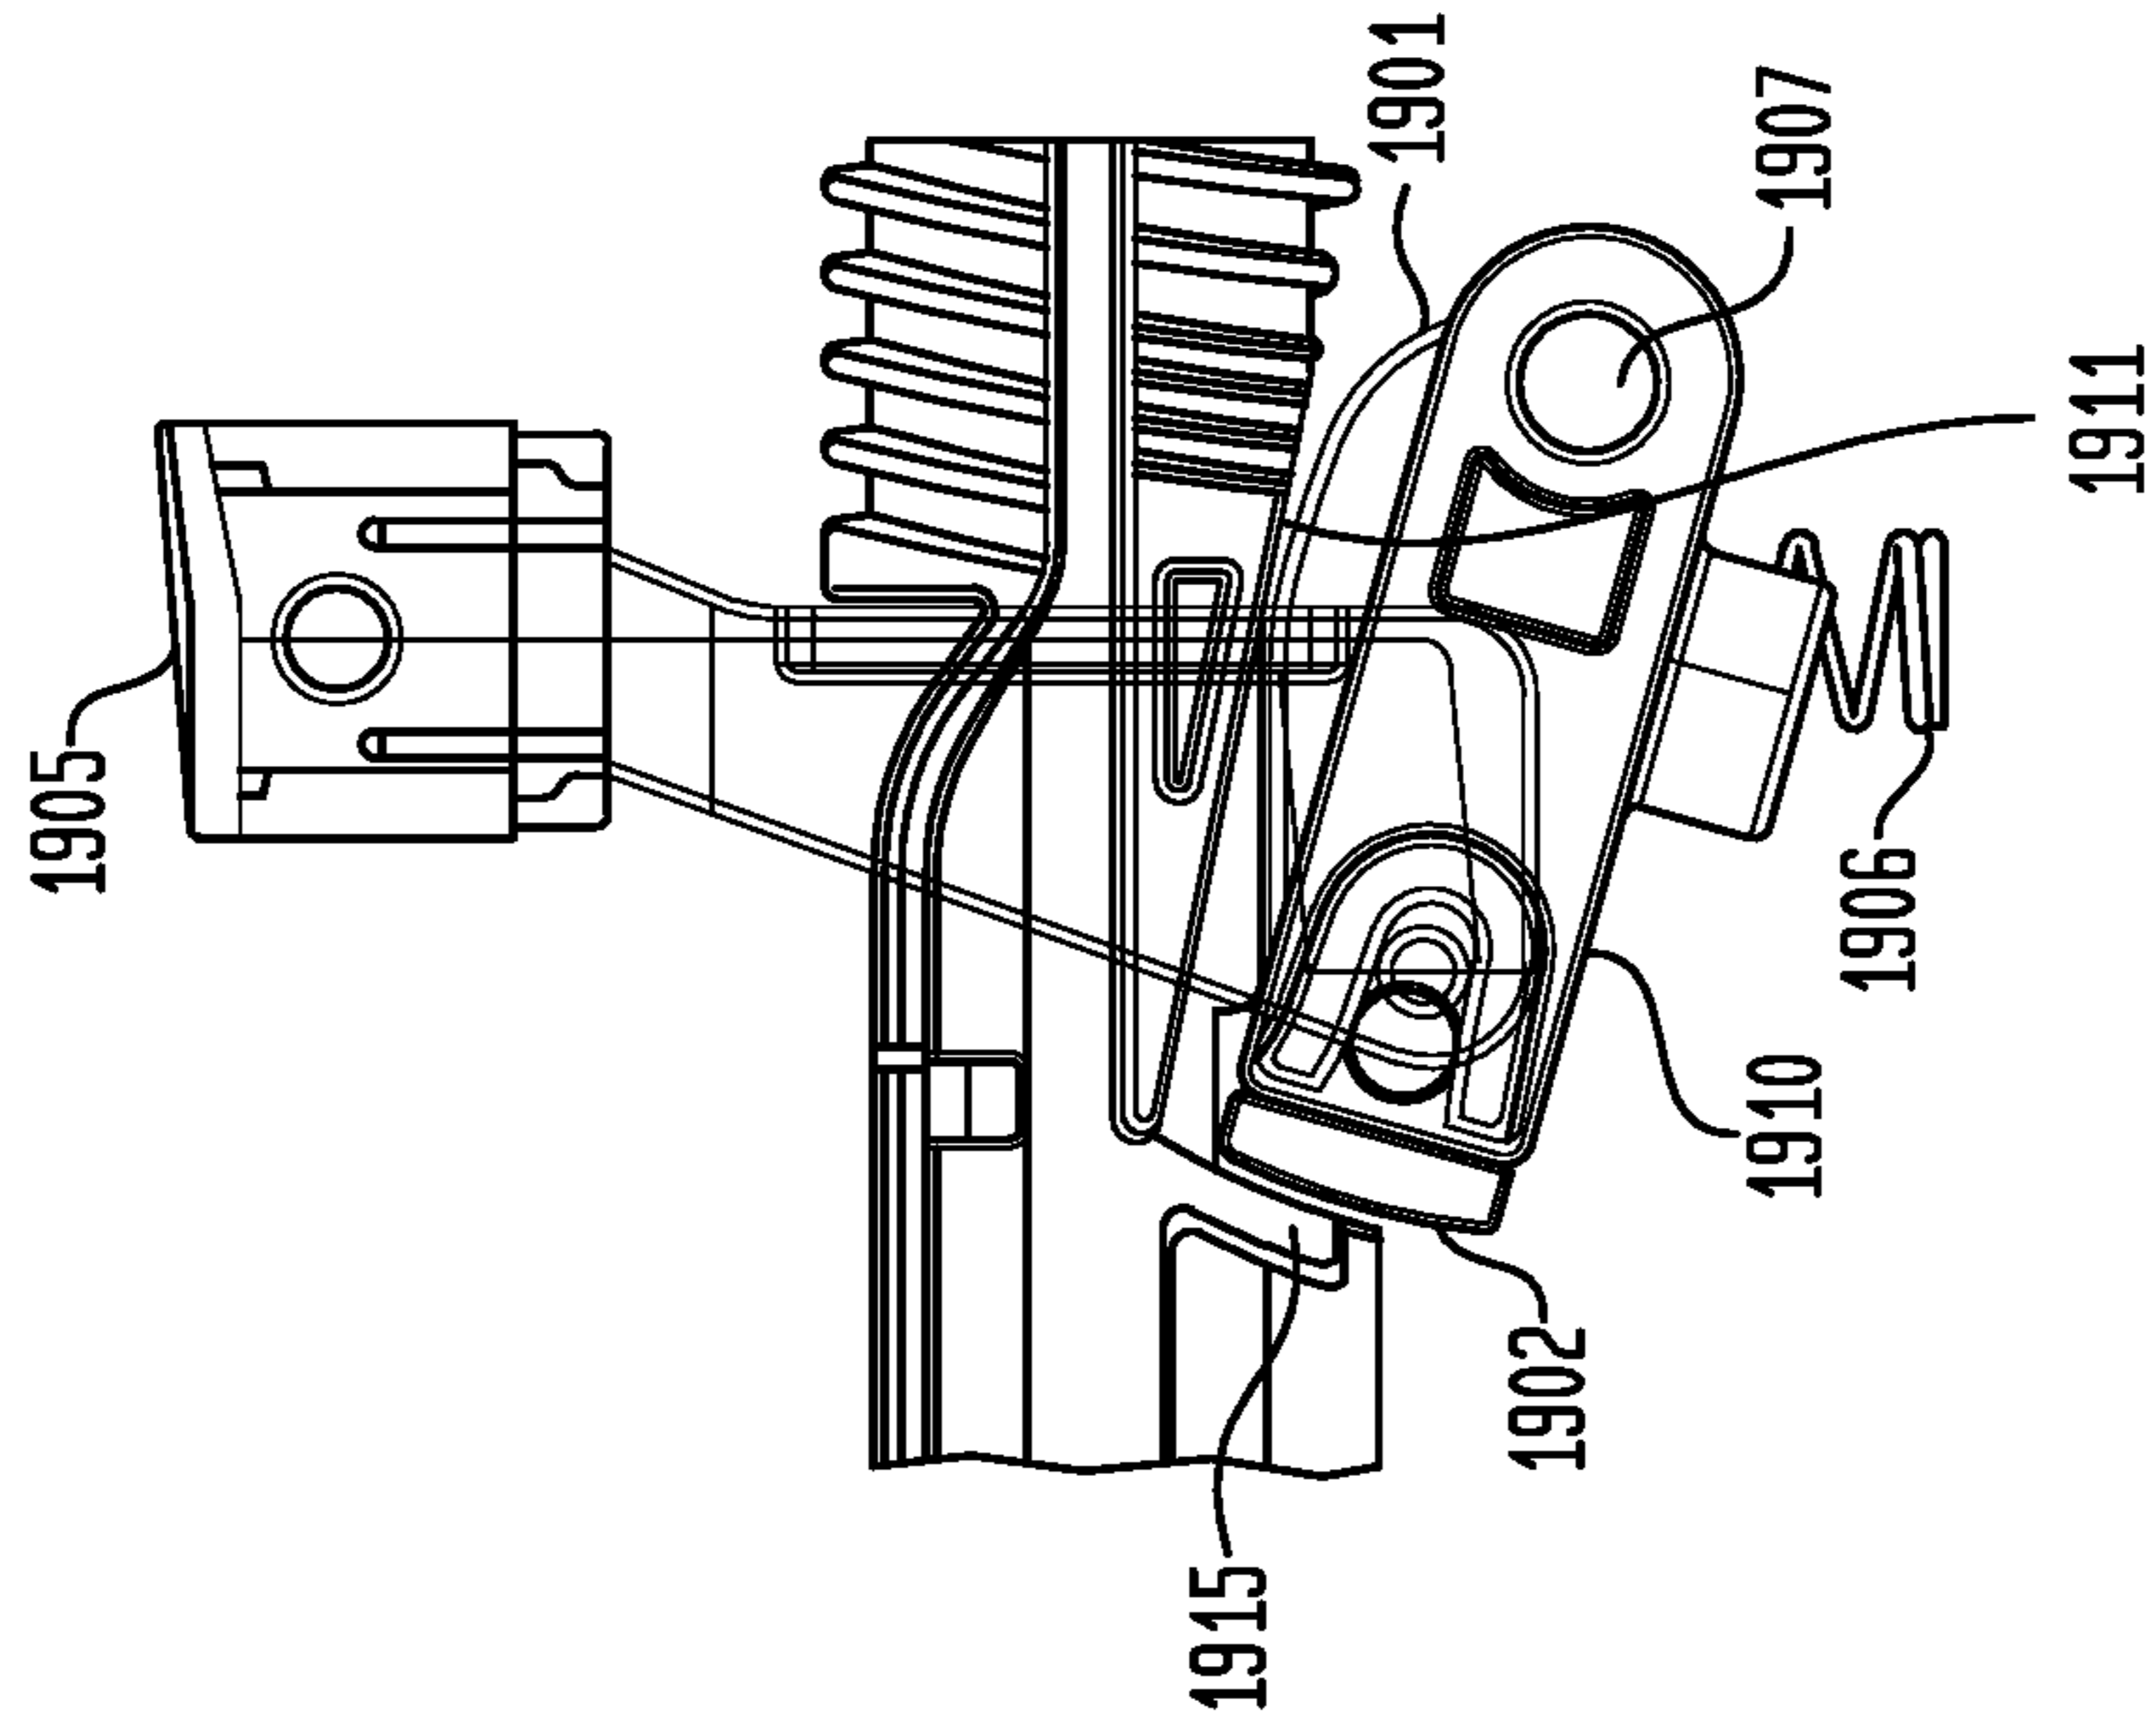

## TRANSCATHETER DELIVERY SYSTEM WITH WHEEL ACTUATION

### CROSS-REFERENCE TO RELATED APPLICATION

The present application claims the benefit of the filing date of U.S. Provisional Patent Application No. 62/506,251 filed May 15, 2017, the disclosure of which is hereby incorporated herein by reference.

### BACKGROUND OF THE INVENTION

The present disclosure relates to a delivery system for heart valve replacement and, in particular, for replacement of collapsible prosthetic heart valves. More particularly, the present disclosure relates to delivery systems for collapsible prosthetic heart valves that may be repositioned during the deployment procedure.

Prosthetic heart valves that are collapsible to a relatively small circumferential size can be delivered into a patient less invasively than valves that are not collapsible. For example, a collapsible valve may be delivered into a patient via a tube-like delivery apparatus such as a catheter, a trocar, a laparoscopic instrument, or the like. This collapsibility can avoid the need for a more invasive procedure such as full open-chest, open-heart surgery.

Collapsible prosthetic heart valves typically take the form of a valve structure mounted on a stent. There are two types of stents on which the valve structures are ordinarily mounted: a self-expanding stent and a balloon-expandable stent. To place such valves into a delivery apparatus and ultimately into a patient, the valve must first be collapsed or crimped to reduce its circumferential size.

When a collapsed prosthetic valve has reached the desired implant site in the patient (e.g., at or near the annulus of the patient's heart valve that is to be replaced by the prosthetic valve), the prosthetic valve can be deployed or released from the delivery apparatus and re-expanded to full operating size. For balloon-expandable valves, this generally involves releasing the entire valve, assuring its proper location, and then expanding a balloon positioned within the valve stent. For self-expanding valves, on the other hand, the stent automatically expands as the sheath covering the valve is withdrawn.

In conventional delivery systems for self-expanding aortic valves, for example, after the delivery system has been positioned for deployment, the annulus end of the valve is typically unsheathed and expanded first, while the aortic end of the valve remains sheathed. Once the annulus end of the valve has expanded, it may be determined that the valve needs to be repositioned in the patient's aortic annulus. To accomplish this, a user (such as a surgeon or an interventional cardiologist) typically resheathes the annulus end of the valve so that the valve can be repositioned while in a collapsed state. After the valve has been repositioned, the user can again release the valve.

Once a self-expanding valve has been fully deployed, it expands to a diameter larger than that of the sheath that previously retained the valve in the collapsed condition, making resheathing difficult. In order for the user to be able to more readily resheath a valve, it is preferable that the valve be only partially deployed, with a portion of the valve still collapsed inside of the sheath.

Despite the various improvements that have been made to the collapsible prosthetic heart valve delivery process, conventional delivery devices, systems, and methods suffer

from some shortcomings. For example, in some delivery devices for self-expanding valves, it is difficult to control how much of the valve remains in the sheath during a partial deployment, and the user may accidentally deploy the valve fully before verifying that the annulus end of the valve is in the optimal position in the patient's valve annulus, thereby taking away the opportunity to resheath and reposition the valve. Moreover, it is difficult during prosthetic heart valve delivery to determine whether a valve assembly will function as intended without full deployment of the heart valve. Due to anatomical variations between patients, a fully deployed heart valve may need to be removed from the patient if it appears that the valve is not functioning properly. Removing a fully deployed heart valve increases the length of the procedure and increases the risk of infection and/or damage to heart tissue.

There therefore is a need for further improvements to the devices, systems, and methods for transcatheter delivery of collapsible prosthetic heart valves, and in particular, self-expanding prosthetic heart valves. Among other advantages, the present disclosure may address one or more of these needs.

### SUMMARY OF THE INVENTION

In some embodiments, a delivery device for a collapsible prosthetic heart valve includes an inner shaft, a distal sheath disposed about a portion of the inner shaft and forming a compartment with the inner shaft, the compartment being adapted to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle including a frame having a longitudinal axis, a proximal end and a distal end, the handle further including a deployment actuator and a hub, each of the deployment actuator and the hub being independently capable of opening and closing the compartment, the hub further including a hub actuator coupled to the inner shaft.

In some embodiments, a delivery device for a collapsible prosthetic heart valve includes an inner shaft, a distal sheath disposed about a portion of the inner shaft and forming a compartment with the inner shaft, the compartment being adapted to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle including a frame having a longitudinal axis, a proximal end and a distal end, the handle further including a deployment actuator a resheathing lock having a lock body coupled to a protruding lock finger in contact with a compression spring, a lock arm coupled to the lock finger, and a lock cap coupled to the lock arm.

In some embodiments, a delivery device for a collapsible prosthetic heart valve includes an inner shaft, a distal sheath disposed about a portion of the inner shaft and forming a compartment with the inner shaft, the compartment being adapted to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle including a frame having a longitudinal axis, a proximal end and a distal end, the handle further including a deployment actuator, the deployment actuator being coupled to a clutch mechanism that permits movement of the distal sheath in a first condition and impedes movement of the distal sheath in a second condition.

### BRIEF DESCRIPTION OF THE DRAWINGS

Various embodiments of the present delivery system are disclosed herein with reference to the drawings, wherein:

FIG. 1 is a side elevational view of a prior art collapsible prosthetic heart valve in an expanded condition, showing the valve assembly attached to the stent;

FIG. 2A is a highly schematic side elevational view showing partial deployment of a collapsible prosthetic heart valve with high placement according to the prior art;

FIG. 2B is a highly schematic side elevational view showing partial deployment of a collapsible prosthetic heart valve with low placement according to the prior art;

FIG. 3A is side view of an operating handle for a transfemoral delivery device for a collapsible prosthetic heart valve, shown with a side elevational view of the distal portion of a transfemoral catheter assembly;

FIGS. 3B-D are side and top views of the operating handle of FIG. 3A, and an enlarged side view of the hub in the proximal-most position, respectively;

FIG. 4 is an enlarged perspective view of the carriage assembly of the handle of FIG. 3A;

FIG. 5 is an enlarged schematic representation of a portion of the threaded rod of the carriage assembly of the operating handle;

FIG. 6 shows a deployment indicator for use with the operating handle;

FIGS. 7A-B are schematic illustrations showing the use of the operating handle of FIG. 3A;

FIG. 8A is a schematic illustration showing the use of a second wheel to close a gap between a distal sheath and a distal tip of a delivery device;

FIGS. 8B-C are longitudinal cross-sectional views of the proximal end of the operating handle of FIG. 3A showing the use of the second wheel to close the gap between the distal sheath and the distal tip of the delivery device;

FIGS. 9A-G are schematic perspective, cross-sectional and side views of another example of a resheathing lock mechanism;

FIG. 10A is a schematic exploded view of an actuator having a clutch mechanism;

FIG. 10B is a longitudinal cross-sectional view of the actuator of FIG. 10A;

FIGS. 10C-D are perspective views of an exemplary drive nut and clutch plate of the actuator of FIG. 10A; and

FIGS. 11A-E are schematic perspective, cross-sectional, front, and side views of another example of a resheathing lock mechanism.

Various embodiments of the present disclosure will now be described with reference to the appended drawings. It is to be appreciated that these drawings depict only some embodiments of the disclosure and are therefore not to be considered limiting of its scope.

#### DETAILED DESCRIPTION

As used herein in connection with prosthetic heart valves, the term “proximal” refers to the end of the heart valve closest to the heart when the heart valve is implanted in a patient, whereas the term “distal” refers to the end of the heart valve farthest from the heart when the heart valve is implanted in a patient. When used in connection with devices for delivering a prosthetic heart valve into a patient, the terms “proximal” and “distal” are to be taken as relative to the user of the delivery devices. “Proximal” is to be understood as relatively close to the user, and “distal” is to be understood as relatively farther away from the user.

FIG. 1 shows a collapsible prosthetic heart valve **200** according to the prior art. The prosthetic heart valve **200** is designed to replace the function of a native aortic valve of a patient. Examples of collapsible prosthetic heart valves are

described in International Patent Application Publication No. WO/2009/042196; and U.S. Pat. Nos. 7,018,406 and 7,329,278, the disclosures of all of which are hereby incorporated herein by reference. As discussed in detail below, the prosthetic heart valve has an expanded condition, shown in FIG. 1, and a collapsed condition. Although the delivery system is described herein in connection with its use to deliver a prosthetic heart valve for replacing a native aortic valve, the delivery system is not so limited, and may be used to deliver prosthetic valves for replacing other types of native or prosthetic cardiac valves.

Prosthetic heart valve **200** includes an expandable stent **202** which may be formed from any biocompatible material, such as metals, synthetic polymers or biopolymers capable of functioning as a stent. Stent **202** extends from a proximal or annulus end **230** to a distal or aortic end **232**, and includes an annulus section **240** adjacent the proximal end and an aortic section **242** adjacent the distal end. The annulus section **240** has a relatively small cross-section in the expanded condition, while the aortic section **242** has a relatively large cross-section in the expanded condition. Preferably, annulus section **240** is in the form of a cylinder having a substantially constant diameter along its length. A transition section **241** may taper outwardly from the annulus section **240** to the aortic section **242**. Each of the sections of the stent **202** includes a plurality of cells **212** connected to one another in one or more annular rows around the stent. For example, as shown in FIG. 1, the annulus section **240** may have two annular rows of complete cells **212** and the aortic section **242** and transition section **241** may each have one or more annular rows of partial cells **212**. The cells **212** in the aortic section **242** may be larger than the cells **212** in the annulus section **240**. The larger cells in the aortic section **242** better enable the prosthetic valve **200** to be positioned without the stent structure interfering with blood flow to the coronary arteries.

Stent **202** may include one or more retaining elements **218** at the distal end **232** thereof, the retaining elements being sized and shaped to cooperate with female retaining structures provided on the deployment device. The engagement of retaining elements **218** with the female retaining structures on the deployment device helps maintain prosthetic heart valve **200** in assembled relationship with the deployment device, minimizes longitudinal movement of the prosthetic heart valve relative to the deployment device during unsheathing or resheathing procedures, and helps prevent rotation of the prosthetic heart valve relative to the deployment device as the deployment device is advanced to the target location and during deployment.

The prosthetic heart valve **200** includes a valve assembly **204** positioned in the annulus section **240**. Valve assembly **204** includes a cuff **206** and a plurality of leaflets **208** which collectively function as a one-way valve. The commissure between adjacent leaflets **208** may be connected to commissure features **216** on stent **202**. FIG. 1 illustrates a prosthetic heart valve for replacing a native tricuspid valve, such as the aortic valve. Accordingly, prosthetic heart valve **200** is shown in FIG. 1 with three leaflets **208**, as well as three commissure features **216**. As can be seen in FIG. 1, the commissure features **216** may lie at the intersection of four cells **212**, two of the cells being adjacent one another in the same annular row, and the other two cells being in different annular rows and lying in end-to-end relationship. Preferably, commissure features **216** are positioned entirely within annulus section **240** or at the juncture of annulus section **240** and transition section **241**. Commissure features **216** may include one or more eyelets which facilitate the suturing of

the leaflet commissure to the stent. However, it will be appreciated that the prosthetic heart valves may have a greater or lesser number of leaflets and commissure features. Additionally, although cuff **206** is shown in FIG. **1** as being disposed on the luminal surface of annulus section **240**, it is contemplated that the cuff may be disposed on the abluminal surface of annulus section **240**, or may cover all or part of either or both of the luminal and abluminal surfaces of annulus section **240**. Both the cuff **206** and the leaflets **208** may be wholly or partly formed of any suitable biological material or polymer.

In operation, a prosthetic heart valve, including the prosthetic heart valve described above, may be used to replace a native heart valve, such as the aortic valve, a surgical heart valve or a heart valve that has undergone a surgical procedure. The prosthetic heart valve may be delivered to the desired site (e.g., near a native aortic annulus) using any suitable delivery device, including the delivery devices described in detail below. During delivery, the prosthetic heart valve is disposed inside the delivery device in the collapsed condition. The delivery device may be introduced into a patient using a transfemoral, transapical or transseptal approach. Once the delivery device has reached the target site, the user may deploy the prosthetic heart valve. Upon deployment, the prosthetic heart valve expands into secure engagement within the native aortic annulus. When the prosthetic heart valve is properly positioned inside the heart, it works as a one-way valve, allowing blood to flow in one direction and preventing blood from flowing in the opposite direction.

In a prosthetic heart valve, the valve assembly may be spaced from the distal or aortic end of the stent by a distance that enables deployment of the heart valve by an amount sufficient for the valve leaflets of the prosthetic valve to operate as intended, while the distal end of the stent remains captured by the delivery device. More particularly, as will be explained further below, the annulus end of the prosthetic heart valve may be deployed first, while the aortic end of the prosthetic heart valve remains at least partially covered by a distal sheath of the delivery device. The annulus portion of the prosthetic heart valve may be deployed so that the entirety of the valve leaflets, up to and including the commissures, is deployed and fully operational. By deploying the prosthetic heart valve in this manner, the user can determine whether the valve leaflets are properly positioned relative to the native valve annulus, and whether the valve is functioning properly. If the user determines that the positioning and operation of the valve are acceptable, the remainder of the valve may be deployed. However, if it is determined that the leaflet position is improper or that the valve is not functioning properly, the user may resheath the valve and either reposition it for redeployment, or remove it entirely from the patient. This can be particularly important in very high risk patients who would typically be recipients of these types of valves because of the nature of their condition and the impact that may have on the shape and/or condition of the native valve and valve annulus.

As is shown in FIG. **1**, in one embodiment the entirety of valve assembly **204**, including the leaflet commissures, is positioned in the annulus section **240** of stent **202**. When opened, the leaflets may extend further into the transition section **241** or may be designed such that they remain substantially completely within the annulus section. That is, substantially the entirety of valve assembly **204** is positioned between the proximal end **230** of stent **202** and the commissure features **216**, and none of the valve assembly **204** is positioned between commissure features **216** and the distal

end **232** of the stent. Indeed, in some embodiments, the valve can be designed such that, upon partial deployment, the commissure features are fully exposed, oriented generally parallel to the direction of blood flow, and at or near their actual radially expanded positions (but not necessarily their eventual positions relative to the annulus), such that the leaflets can operate substantially as they would when the valve is fully deployed, even though enough of the stent is still retained within the delivery device or sheath to permit resheathing.

In a preferred arrangement, the distance between commissure features **216** and the distal end **232** of stent **202** will be about two-thirds of the length of the stent from the proximal end **230** to the distal end. This structural arrangement provides advantages in the deployment of prosthetic valve **200** as will be discussed in more detail with reference to FIGS. **2A** and **2B**. By having the entirety of valve assembly **204** positioned within annulus section **240**, and by having a sufficient distance between commissure features **216** and the distal end **232** of stent **202**, the valve assembly and commissures will not impede blood flow into the coronary arteries and will not interfere with access thereto during cardiac intervention, such as angiography, annuloplasty or stent placement.

Further, it is possible to partially deploy prosthetic valve **200** so that the valve assembly **204** thereof is able to fully function in its intended position in the native valve annulus, while a sufficient amount of the aortic section **242** is retained within the delivery device should resheathing become necessary. In other words, as will be explained in more detail below, the user may withdraw the distal sheath of the delivery device to gradually expose prosthetic valve **200**, beginning at the proximal end **230**. Continued withdrawal of the distal sheath will expose a greater extent of the prosthetic valve until the entire annulus section **240** and valve assembly **204** have been exposed. Upon exposure, these portions of the prosthetic valve will expand into engagement with the native valve annulus, entrapping the native valves, except for a small portion immediately adjacent the free end of the distal sheath which will be constrained by the distal sheath from fully expanding.

However, once the distal sheath has been withdrawn to expose a sufficient portion of the aortic section **242**, the annulus section **240** will be able to fully expand and valve assembly **204** will be able to function in the same manner as if the entirety of prosthetic valve **200** had been deployed. At this juncture, it will be possible for the user to ascertain whether annulus section **240** and valve assembly **204** have been properly positioned relative to the native valve annulus, and whether the valve assembly is functioning properly.

If the position and operation of valve assembly **204** are acceptable, the distal sheath may be withdrawn further to deploy the remainder of prosthetic valve **200**. On the other hand, if the positioning or operation of valve assembly **204** are unacceptable, the user may advance the distal sheath to resheath the prosthetic valve, reposition the valve and initiate the deployment procedure anew. And if it is determined that the valve is not functioning properly, it can be withdrawn from the patient and a new valve introduced.

It will be appreciated from the foregoing that the placement of the leaflets **208** within the stent **202** can affect the valve functioning during partial deployment. FIG. **2A** illustrates a valve assembly **204** with high placement, while FIG. **2B** illustrates a valve assembly with low placement. As used herein, the phrase "high placement" of a valve assembly refers to locating the valve assembly within the transition section **241** of the stent **202**, or within the portion of the

annulus section **240** closest to the transition section. The phrase “low placement” of a valve assembly refers to locating the valve assembly closer to the proximal end **230** of the stent **202** and entirely within the annulus section **240** thereof, such that the leaflets **208** are substantially disposed within the annulus section.

As seen in FIG. 2A, during partial deployment the annulus end of the heart valve **200** is unsheathed and allowed to expand. The distal end **232**, including the aortic section **242**, remains partially sheathed and coupled to the delivery device. Operation of the delivery device is described below in more detail with reference to FIGS. 3A-7B. Turning back to FIG. 2A, it will be appreciated that high placement of valve assembly **204** will cause the valve assembly to not be fully deployed when heart valve **200** is only partially deployed, thereby affecting leaflet function. Specifically, since the commissure features **216** are located closer to or within the transition section **241**, they do not reach their fully expanded positions. As such, the leaflets **208** remain partially closed at this stage of deployment. Because of the location of the commissure features **216** and the leaflets **208**, the valve assembly **204** cannot be tested during partial deployment. Instead, the user must unsheath a portion of the aortic section **242** as well, which may pose problems if the valve assembly **204** is to be resheathed and redeployed.

In contrast to the prosthetic heart valve of FIG. 2A, the heart valve **200** of FIG. 2B exhibits low placement of the valve assembly **204** within the annulus section **240**. Low placement of the valve assembly **204** enables the valve assembly to fully deploy when heart valve **200** is only partially deployed. As such, leaflets **208** reach their fully expanded and open positions during partial deployment and are able to function near normally, enabling a better assessment of the valve’s functioning and final placement within the actual anatomy. Thus, if it appears that the valve needs to be moved, the heart valve **200** may be easily resheathed and repositioned. This concept is beneficial when dealing with less than ideal anatomical configurations.

The shape of the stent **202** during partial deployment will also affect the valve **204**. If the stent shape is such that, while still partially retained by the sheath, it cannot open sufficiently to allow operation of the valve, it may not be possible to fully assess the operation of the valve in its intended placement position. Moreover, the height of the valve commissure features **216** relative to the proximal end **230** of the valve will affect the valve function. The lower the commissure features **216**, meaning the closer to the proximal end **230**, the more they will expand outwardly and the valve leaflets will be able to open during partial deployment, creating a flow passageway through the leaflets which approaches that of a fully deployed valve.

A transfemoral or transapical delivery device may be used to partially deploy the prosthetic heart valve such that an assessment may be made regarding flow through the valve and adequacy of coaptation. If, after the annulus section is unsheathed and the valve is tested, it is found that the valve needs to be repositioned, the annulus section may be resheathed and the valve redeployed as necessary.

Turning now to FIGS. 3A-D, an exemplary transfemoral delivery device **1010** for a collapsible prosthetic heart valve (or other types of self-expanding collapsible stents) has a catheter assembly **1016** for delivering the heart valve to and deploying the heart valve at a target location, and an operating handle **1020** for controlling deployment of the valve from the catheter assembly. The delivery device **1010** extends from a proximal end **1012** to a distal tip **1014**. The catheter assembly **1016** is adapted to receive a collapsible

prosthetic heart valve (not shown) in a compartment **1023** defined around an inner shaft **1026** and covered by a distal sheath **1024**. The inner shaft **1026** extends through the operating handle **1020** to the distal tip **1014** of the delivery device, and includes a retainer **1025** affixed thereto at a spaced distance from distal tip **1014** and adapted to hold a collapsible prosthetic valve in the compartment **1023**.

The distal sheath **1024** surrounds the inner shaft **1026** and is slidable relative to the inner shaft such that it can selectively cover or uncover the compartment **1023**. The distal sheath **1024** is affixed at its proximal end to an outer shaft **1022**, the proximal end of which is connected to the operating handle **1020** in a manner to be described. The distal end **1027** of the distal sheath **1024** abuts the distal tip **1014** when the distal sheath fully covers the compartment **1023**, and is spaced apart from the distal tip **1014** when the compartment **1023** is at least partially uncovered.

The operating handle **1020** is adapted to control deployment of a prosthetic valve located in the compartment **1023** by permitting a user to selectively slide the outer shaft **1022** proximally or distally relative to the inner shaft **1026**, or to slide the inner shaft **1026** relative to the outer shaft **1022**, thereby respectively uncovering or covering the compartment with the distal sheath **1024**. Operating handle **1020** includes frame **1030** which extends from a proximal end **1031** to a distal end and includes a top frame portion **1030a** and a bottom frame portion **1030b**. The proximal end of the inner shaft **1026** is coupled to a hub **1100**, and the proximal end of the outer shaft **1022** is affixed to a carriage assembly **1040** (FIG. 4) that is slidable within the operating handle along a longitudinal axis of the frame **1030**, such that a user can selectively slide the outer shaft relative to the inner shaft by sliding the carriage assembly relative to the frame. Alternatively, inner shaft **1026** may be actuated via hub **1100** to cover or uncover the compartment as will be discussed in greater detail below. Optionally, a stability sheath **1051** is disposed over some or all of outer shaft **1022**. The stability sheath **1051** may be attached to the outer shaft **1022** or may be unattached. Additionally, stability sheath **1051** may be disposed over a majority of outer shaft **1022** or over a minority of the outer shaft (e.g., over 49% or less, over 33%, etc.). Optionally, stability sheath **1051** may be more rigid than outer shaft **1022**.

Additionally, hub **1100** may include a pair of buttons **1610**, each attached to a clip **1612** (FIG. 3D). Clips **1612** on hub **1100** may mate with voids **1614** on frame **1030** to ensure that the hub and the frame are securely coupled together. Optionally, hub **1100** may also include a wheel **1600**, which will be described in greater detail below.

A first mechanism for covering and uncovering the compartment **1023** will be referred to as a “fine” technique as covering and uncovering occurs slowly with a high degree of precision. To allow for this technique, frame **1030** defines an elongated space **1035** in which carriage assembly **1040** may travel (FIG. 5). The elongated space preferably permits the carriage assembly **1040** to travel a distance that is at least as long as the anticipated length of the prosthetic valve to be delivered (e.g., at least about 50 mm), such that the distal sheath **1024** can be fully retracted off of the prosthetic valve.

The carriage assembly **1040** includes a main body **1041** and a threaded rod **1036** extending proximally therefrom along the longitudinal axis of the frame **1030**. The threaded rod **1036** preferably is longer than the anticipated maximum travel distance of the carriage assembly **1040** within the elongated space **1035** (e.g., at least about 50 mm), such that the threaded rod does not fully withdraw from the elongated space **1035** during deployment of the prosthetic valve.



A deployment actuator **1021**, shown in FIGS. 3A-D as a wheel protruding from the upper and lower frames **1030a**, **1030b** is fixedly coupled to a first gear **1037** so that rotation of actuator **1021** causes a corresponding rotation of gear **1037**. Gear **1037**, in turn, is threadedly engaged on the threaded rod **1036**. Gear **1037** converts rotation of deployment actuator **1021** into longitudinal translation of threaded rod **1036** in the direction of arrows T1 and T2 and a corresponding translation of main body **1041**. Hence, rotation of actuator **1021** in one direction (either clockwise or counterclockwise depending on the orientation of the threads on the threaded rod **1036**) causes the carriage assembly **1040** to translate proximally in direction T1 within the elongated space **1035**. Alternatively, actuator **1021** and first gear **1037** may be integral with one another.

As outer shaft **1022** is fixedly connected to carriage assembly **1040**, translation of the carriage assembly results in a longitudinal translation of outer shaft **1022** and with it distal sheath **1024**. Thus, deployment actuator **1021** is configured to provide for fine movement of outer shaft **1022** for deployment and recapture of the prosthetic heart valve. As deployment actuator **1021** protrudes from upper and lower frames **1030a**, **1030b** approximately halfway between the proximal and distal ends of the handle **1020**, a user may readily rotate the actuator with his or her thumb and/or index finger (FIG. 7A).

Optionally, handle **1020** further includes a resheathing lock **1043** adapted to prevent any movement of the carriage assembly within the frame **1030**, thereby preventing a user from accidentally initiating deployment of a prosthetic valve (FIG. 3C). Resheathing lock **1043** may be coupled to the main body **1041** of carriage assembly **1040**. The resheathing lock **1043** may include a laterally projecting pin **1044** that is slidable within a hole **1046** in main body **1041**. Pin **1044** may have a first or unlocked condition in which it is compressed between main body **1041** and frame **1030**.

As the user rotates deployment actuator **1021**, outer shaft **1022** is pulled back and with it distal sheath **1024** to uncover a portion of compartment **1023**. This process may continue until a predetermined position just prior to a position at which resheathing is no longer possible. When this predetermined position is reached, a spring **1045** positioned in hole **1046** between main body **1041** and pin **1044** pushes the pin out through an aperture in frame **1030** to a second or locked condition (FIG. 5) in which the pin protrudes from frame **1030**, providing a visual indicator to the user that resheathing is no longer possible past this predetermined position. Further translation of the carriage assembly **1040** may be impeded until the user presses pin **1044** to the interior of frame **1030** against the action of spring **1045** to confirm that further uncovering of compartment **1023** is desired (i.e., that the user wishes to fully deploy the prosthetic heart valve in its current position).

The initial distance that the carriage assembly **1040** can travel before actuating resheathing lock **1043** may depend on the structure and size of the particular prosthetic valve to be deployed. Preferably, the initial travel distance of the carriage assembly **1040** is about 3 mm to about 5 mm less than the length of the valve in the collapsed condition (e.g., about 3 mm to about 5 mm of the valve may remain covered to permit resheathing). Alternatively, the initial travel distance of the carriage assembly **1040** may be about 40 mm to about 45 mm, which is about 80% to about 90% of the length of an exemplary 50 mm valve. In other arrangements, the initial distance that the carriage assembly **1040** can travel can be determined as a percentage of the length of the prosthetic valve in the collapsed condition and/or of the

compartment **1023**, including, for example, 50%, 60%, 70%, 75%, 85%, 95% or anywhere between about 50% and about 95%. Thus, resheathing lock **1043** may allow uncovering of compartment **1023** up to a maximum distance or percentage, and allow further uncovering only after the user has pressed on laterally projecting pin **1044** to confirm that additional release (e.g., full release of the prosthetic heart valve) is desired.

A second technique, referred to as a "coarse technique," may be used to cover and uncover compartment **1023** more quickly and with less precision than the fine technique described above. Specifically, hub **1100** may be coupled to the proximal end of inner shaft **1026** and may be capable of moving the inner shaft relative to frame **1030** to facilitate opening and closing of the compartment **1023**. This coarse movement may be used when no prosthetic heart valve is present in the compartment, such as, for example, when the compartment is to be opened prior to loading the prosthetic heart valve, and when the compartment is to be closed after the valve has been fully deployed. A mechanical lock **1110** may couple hub **1100** to frame **1030** to prevent accidental movement during use of operating handle **1020**. For example, hub **1100** and a portion of frame **1030** may be threadedly engaged such that a rotation of the hub relative to the frame is required to release the hub from the frame. Other types of mechanical locks that will releasably couple hub **1100** to frame **1030** as intended will be known to those skilled in the art. After lock **1110** has been disengaged, hub **1100** may be used to quickly cover or uncover compartment **1023**. Movement of inner shaft **1026** with respect to outer shaft **1022** may open and close the compartment. Thus, pushing hub **1100** distally (and thus the distal movement of inner shaft **1022**) opens compartment **1023** and pulling hub **1100** proximally closes the compartment.

Optionally, an indicator window **1500** (FIG. 6) may be disposed on top of frame **1030** and may include a series of increments **1510** showing a percent or extent of deployment of the prosthetic heart valve. A scrolling bar **1520** may move along window **1500** past the series of increments **1510** as deployment continues to illustrate to the user the extent to which the prosthetic heart valve has been deployed. As illustrated, scrolling bar **1520** indicates that a prosthetic heart valve is approximately 37.5% deployed. Indicator window **1500** further includes a critical indicator **1530** showing the position past which resheathing is no longer possible. Resheathing lock **1043** may be activated as scrolling bar **1520**, which is coupled to the main body **1041** of carriage assembly **1040** reaches position **1530**.

The general operation of the delivery device **1010** to deploy a prosthetic valve will now be described. Device **1010** may be shipped with outer shaft **1022** in its proximal-most position. Hub **1100** may also be initially shipped in a proximal-most position, the hub being spaced away from frame **1030**. (FIG. 7B) However, compartment **1023** will be covered by distal sheath **1024**. To load the delivery device **1010** with a collapsible prosthetic valve, a user can push hub **1100** distally (and advance inner shaft **1026**) to expose the compartment **1023** (FIG. 7A), thread the inner shaft **1026** through the valve, collapse the valve and couple it to a retainer, and rotate deployment actuator **1021** to advance the distal sheath back over compartment **1023** to fully cover the valve. In this starting condition, the handle **1020** will be in an initial state with the carriage assembly **1040** at its distal-most position within the frame **1030**, the resheathing lock **1043** will be in an unlocked state with pin **1044** disposed within frame **1030**, the hub **1100** will be in its

## 11

distal-most position and coupled to frame 1030, and the deployment indicator will show 0% deployment.

To use the operating handle 1020 to deploy the prosthetic valve, the user can rotate the deployment actuator 1021, causing the carriage assembly 1040 to slide proximally within the elongated space 1035 in frame 1030. Because the distal sheath 1024 is affixed to the outer shaft 1022, which in turn is affixed to the carriage assembly 1040, sliding the carriage assembly proximally relative to the frame will cause the distal sheath to move proximally. Since the inner shaft 1026 is at this point fixed to frame 1030, it will not move. Hence, the proximal movement of distal sheath 1024 relative to inner shaft 1026 will uncover the compartment 1023, thereby exposing and initiating deployment of the valve located therein.

Movement of the carriage assembly 1040 proximally may continue only until the resheathing lock 1043 is actuated and pin 1044 protrudes from frame 1030. At this point, the distal sheath 1024 will not be fully withdrawn from around the compartment 1023, and the prosthetic valve will not be fully deployed. Moreover, indicator window 1500 will show that scrolling bar 1520 has reached critical indicator 1530 and that any further uncovering of the compartment will fully deploy the prosthetic heart valve and prevent its resheathing.

When the deployment procedure has reached this juncture, the user can evaluate the position of the valve and determine whether the annulus end of the valve is properly aligned relative to the patient's native valve annulus. If repositioning is desired, the user may resheath the valve by using deployment actuator 1021 to slide the carriage assembly 1040 distally within the frame 1030, thereby moving the distal sheath 1024 distally over the compartment 1023 and over the partially deployed valve to recollapse the expanded portion of the valve. With the valve resheathed, the user can reposition the catheter assembly 1016 and commence the deployment procedure once again.

Once the valve has been properly positioned relative to the aortic annulus, the user may complete the deployment process. To do so, the user presses pin 1044 through the aperture in frame 1030, releasing lock 1043, which frees carriage assembly 1040 to continue its movement proximally within the frame. The user can complete the deployment of the valve by continuing to slide the carriage assembly 1040 proximally, for example, by rotating the deployment actuator 1021. When the valve has been fully unshathed, the stent portion of the valve self-expands and disengages from the retainer 1025, thereby releasing the valve from the catheter assembly 1016, following valve deployment, hub 1100 may once again be used to quickly cover the compartment and the delivery device may be removed from the patient.

Three additional features may be added to the delivery device 1010 described above to improve the performance of the device. It will be understood that all three of these features are optional, and that the delivery device may include none of the features, one of the features, or a combination of the features as desired. The three features are the optional use of a second wheel for gap closure, a robust resheathing lock mechanism, and an actuator clutch mechanism. Each will be described, in turn, with reference to FIGS. 8-10.

FIGS. 8A-C illustrate the use of additional features on the hub 1100 to aid in valve loading and delivery. As discussed, the delivery device 1010 may be packaged with the hub 1100 withdrawn to the proximal position and the deployment actuator 1021 turned such that the distal sheath 1024 is in its proximal position, leaving a closed capsule (see FIG. 3A).

## 12

Hub 1100 may be moved distally to move inner shaft 1026 to its distal position and thus open the compartment 1023 for valve loading. After the valve has been loaded, actuator 1021 may be rotated to move the distal sheath 1024 over the valve and close the compartment 1023. The delivery device 1010 is designed such that the distal end 1027 of the distal sheath 1024 abuts the distal tip 1014 when the distal sheath fully covers the compartment 1023, and is spaced apart from the distal tip 1014 when the compartment 1023 is at least partially uncovered.

As shown in FIG. 8A, in some circumstances, though the actuator 1021 has been properly used to close the compartment 1023, the distal end 1027 of the distal sheath 1024 may not abut the distal tip 1014, leaving a gap g1 between the distal end of the sheath and the distal tip 1014. This gap may be due to residual compression in distal sheath 1024 and/or frictional forces between distal sheath 1024 and the loaded prosthetic heart valve. In effect, though distal sheath 1024 has been fully moved to its distal-most position with respect to the shaft 1026, it may be slightly bunched together and not fully extended, leaving gap g1.

To close the gap g1, a second wheel 1600 may be used, the details of which are shown in FIGS. 8B-C. Wheel 1600 may be disposed in hub 1100 and mounted over cam 1605 having threaded portion 1606, cam 1605 in turn being coupled to inner shaft 1026. Turning wheel 1600 while holding frame 1030 may pull cam 1605, and thus inner shaft 1026, proximally to close the gap g1 and force the distal end 1027 of distal sheath 1024 to abut distal tip 1014 (FIG. 8C). Once the gap g1 is closed, wheel 1600 may be rotated in the opposite direction to relieve any tension within the distal sheath 1024 (FIG. 8B). A flange 1607 on cam 1605 may contact wheel 1600 and create a hard stop position when returning inner shaft 1026 to a neutral position. In some embodiments, wheel 1600 allows for translation of shaft 1026 by between about 0.25 inch and about 1 inch relative to distal sheath 1024.

FIGS. 9A-G illustrate another example of a resheathing lock mechanism 1700. As shown in FIGS. 9A-B, resheathing lock mechanism 1700 generally includes a lock body 1701 having of two ribs that face one another and lock finger 1702 that sits on compression spring 1703 and protrudes from the lock body in the distal direction. Lock body 1701 is coupled to lock arms 1704, which in turn are coupled to a lock button 1705 that protrudes from frame 1030. A dowel hinge pin 1707 pivotally connects lock body 1701 to frame 1030. A leaf spring 1706 extending from the base of lock body 1701 and fixed to the frame 1030 is configured to apply a constant upward force to lock body 1701.

As shown in FIGS. 9C-D, ribs of the lock body 1701 are disposed in elongated slots 1710 formed on opposite sides of threaded rod 1036. As the actuator 1021 is operated to move carriage assembly 1040 with respect to lock mechanism 1700, the ribs ride along slots 1710 in the threaded rod 1036. At or near the distal end of the threaded rod 1036, each of the slots includes a ramp 1711 that angles upward toward the upper portion of frame 1030 (not shown). As the carriage assembly 1040 and threaded rod 1036 move proximally, the ribs of lock body 1701 continue to ride along the slots 1710 in threaded rod 1036 and up ramp 1711 as the lock body is urged to pivot upward by leaf spring 1706 (FIG. 9D).

The upward movement of the lock body 1701 moves lock finger 1702 upward toward carriage assembly 1040, wherein it is eventually received in a cavity 1715 formed in the carriage assembly (FIG. 9E). As the carriage assembly continues to move proximally with rotation of the actuator 1021, lock finger 1702 contacts an end wall of cavity 1715

## 13

such that for the retraction of the carriage assembly gradually compresses spring 1703. When spring 1703 is fully compressed, carriage assembly 1040 is mechanically locked against further travel (FIG. 9F). This locked position corresponds to the point past which resheathing of the heart valve is no longer possible. The user may test functionality of the valve at this point, resheath and re-implant the valve, or remove the prosthetic heart valve entirely. If the physician decides to continue the procedure and release the valve entirely, lock button 1705 may be depressed, pivoting the lock body 1701 and lock finger 1702 downward until lock finger 1702 no longer contacts the end wall of cavity 1715. At this point, spring 1703 may force lock finger 1702 outward and below carriage assembly 1040, releasing the carriage assembly for further proximal movement (FIG. 9G).

The actuator 1021 of the delivery device 1010 may also include a clutch mechanism so that when the resheathing lock 1700 is engaged, if the user continues to rotate the actuator a clutch between the actuator and the threaded rod 1036 prevents damage to the device. FIG. 10A shows one example of a clutch mechanism for use with actuator 1021. As shown, a clutch plate 1804 is assembled in a shell 1801 of actuator 1021 with a compression spring 1805 disposed between the clutch plate and the shell. In its assembled position, features (not shown) on the clutch plate 1804 engage with corresponding features (not shown) in the interior of shell 1801 to rotationally lock the clutch plate to the shell but permit the clutch plate to move axially within the shell. A drive nut 1803 is positioned adjacent clutch plate 1804, and the entire assembly is enclosed by a wheel cap 1802. A pair of assembly screws 1806 assemble the wheel cap 1802 to the wheel shell 1801 to hold the assembly together. Drive nut 1803 is internally threaded so that the fully assembled actuator 1021 may be threaded onto threaded rod 1036. Drive nut 1803 is not rotationally locked to shell 1801 but rather is freely rotatable relative to same. A cross-sectional view of the assembled actuator 1021 mounted on threaded rod 1036 is shown in FIG. 10B.

Details of drive nut 1803 and clutch plate 1804 will be described in greater detail with reference to FIGS. 10C and 10D. Drive nut 1803 includes a plurality of directional teeth 1813 around its circumference, each tooth having a sloped portion 1814 and a generally perpendicular portion 1815. The teeth 1813 on drive nut 1803 confront a plurality of complementary directional teeth 1816 positioned around the circumference of clutch plate 1804. Directional teeth 1816 have a similar configuration to the teeth 1813 of the drive nut 1803 so that the teeth are able to mesh with one another. When a predetermined axial force is reached upon rotation of the actuator 1021 in the deployment direction, teeth 1813 and 1816 slip relative to one another in a first direction. Compression spring 1805 applies a constant engagement force to keep clutch plate 1804 engaged with drive nut 1803 until the predetermined force is reached. Slippage occurs when a force greater than the predetermined force is applied, which typically occurs when the actuator is rotated while the resheathing lock mechanism 1700 is in the locked position. The predetermined slippage force may be determined by the angle of the sloped portion of teeth 1813 and 1816, the height of the teeth (i.e., the height of the perpendicular portions), spring force of compression spring 1805, and friction between drive nut 1803 and clutch plate 1804.

In use, resheathing lock mechanism 1700 may be urged toward the locked position as described above, preventing the carriage assembly 1040 from moving further in the proximal direction. As carriage assembly 1040 is unable to

## 14

move proximally, drive nut 1803 also will be unable to move as actuator 1021 is rotated in the direction causing proximal movement of the carriage assembly. The continued effort to rotate actuator 1021 will eventually result in the exerting of the predetermined force on the actuator. When this force is reached, the rotational force on the wheel shell 1801 will drive the clutch plate teeth 1816 up the sloped portion 1814 of the teeth of the drive nut 1803, moving the clutch plate 1804 axially until the teeth slip relative to one another. Thus, wheel shell 1801 will be allowed to rotate without any movement of carriage assembly 1040 and without exerting excessive force on the resheathing lock mechanism 1700 that could potentially damage same. In effect, this clutch mechanism serves to limit the amount of force that the user can apply to the resheathing lock mechanism 1700 and also provides a user input that the partial deployment limit has been reached when the user senses that the wheel is turning but no further actuation results. During re-sheathing of the valve, where the forces on the catheter are highest, in a direction opposite the first direction, the teeth are engaged in such a manner as to prevent any slippage of the clutch due to the presence of generally perpendicular portions 1815 on the teeth.

FIGS. 11A-E illustrate another example of a resheathing lock mechanism 1900, which is a variation of the resheathing lock mechanism 1700 shown in FIGS. 9A-G. The resheathing lock mechanism 1900 has an identical structure and function to the resheathing lock mechanism 1700, except for the differences that are described below. As shown in FIGS. 11A-B, resheathing lock mechanism 1900 generally includes a lock body 1910 having two ribs 1901 that face one another and lock finger 1902 that sits on compression spring 1903 and protrudes from the lock body in the distal direction. Lock body 1910 is coupled to lock arms 1904, which in turn are coupled to a lock button 1905 that is configured to protrude through an opening in frame 1030 when in a locked condition. A dowel hinge pin 1907 pivotally connects lock body 1910 to frame 1030. A compression spring 1906 (e.g., a coil spring) extending from the base of lock body 1910 and fixed to frame 1030 is configured to apply a constant upward force to lock body 1910. In some embodiments, a torsion spring may be used in place of compression spring 1906.

As shown in FIGS. 11C-D, ribs 1901 of the lock body 1910 maintain contact with the bottom of threaded rod 1036 due to the force provided by compression spring 1906. As actuator 1021 is operated to move carriage assembly 1040 and threaded rod 1036 with respect to lock mechanism 1900, the threads of the threaded rod slide along ribs 1901, with the ribs oriented transverse (e.g., 80°-85°) to the threads. At or near the distal end of threaded rod 1036, the threaded rod defines a cavity 1915 formed in the bottom of carriage assembly 1040. Cavity 1915 defines a ramp 1911 (FIG. 11E) that angles upward toward the upper portion of frame 1030 (not shown). As the carriage assembly 1040 and threaded rod 1036 move proximally, ribs 1901 of lock body 1910 continue to ride along the bottom of threaded rod 1036 and up ramp 1911 as the lock body is urged to pivot upward about dowel hinge pin 1907 by compression spring 1906.

The upward pivoting of the front of lock body 1910 moves lock finger 1902 upward toward carriage assembly 1040, wherein it is eventually received in cavity 1915. As carriage assembly 1040 continues to move proximally with the rotation of actuator 1021, lock finger 1902 contacts an end wall of cavity 1915 such that continued proximal translation of the carriage assembly gradually compresses spring 1903. When spring 1903 is fully compressed, carriage

15

assembly 1040 is mechanically locked against further proximal travel (FIG. 11E). This locked position corresponds to the point past which resheathing of the heart valve is no longer possible. The user may test functionality of the valve at this point, resheath and re-implant the valve, or remove the prosthetic heart valve entirely. If the physician decides to continue the procedure and release the valve entirely, lock button 1905 may be depressed, pivoting lock body 1910 and lock finger 1902 downward until the lock finger no longer contacts the end wall of cavity 1915. At this point, spring 1903 forces lock finger 1902 distally below carriage assembly 1040, releasing the carriage assembly for further proximal movement, in a manner similar to that shown in FIG. 9G.

In some examples, a delivery device for a collapsible prosthetic heart valve, the delivery device includes an inner shaft, a distal sheath disposed about a portion of the inner shaft to form a compartment with the inner shaft, the compartment being sized to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle including a frame having a longitudinal axis, a deployment actuator operatively connected to the distal sheath, and a hub operatively connected to the inner shaft, each of the deployment actuator and the hub being independently capable of opening and closing the compartment, the hub further including a hub actuator coupled to the inner shaft; and/or the deployment actuator includes a first wheel having an axis of rotation disposed parallel to the longitudinal axis of the frame, and the hub actuator includes a second wheel having an axis of rotation that is parallel to the axis of rotation of the first wheel; and/or the second wheel is engaged with a translating cam having a threaded portion, the cam being coupled to the inner shaft; and/or the cam includes a flange that is perpendicular to the axis of rotation of the second wheel; and/or the cam is capable of translating between about 0.25 inches and about 1 inch in a direction parallel to the axis of rotation of the second wheel; and/or rotation of the second wheel results in longitudinally translating the inner shaft; and/or rotation of the deployment actuator results in longitudinally translating the distal sheath to cover or uncover the compartment.

In some examples, a delivery device for a collapsible prosthetic heart valve, the delivery device includes an inner shaft, a distal sheath disposed about a portion of the inner shaft to form a compartment sized to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle including a frame having a longitudinal axis, a deployment actuator a resheathing lock having a lock body coupled to a protruding lock finger in contact with a compression spring, a lock arm coupled to the lock finger, and a lock button coupled to the lock arm; and/or the lock button has a first position disposed within the frame, and a second position in which the lock button protrudes from the frame; and/or the distal sheath is coupled to a threaded rod, the threaded rod being coupleable to the lock body; and/or the threaded rod includes a slot having a ramp and the lock body slides within the slot of the threaded rod; and/or the lock body has a pair of ribs configured to maintain contact with a bottom of the threaded rod when the threaded rod translates along the longitudinal axis of the frame; and/or the lock finger is configured to be disposed within a cavity of threaded rod in a first lock condition that prevents distal movement of the distal sheath, and to be substantially parallel with the threaded rod in a second unlocked condition that allows distal movement of the distal sheath; and/or the delivery device further includes a leaf spring coupled to the lock finger; and/or the leaf spring

16

is configured to apply a force to the lock body; and/or the delivery device further includes a compression spring coupled to the lock finger; and/or the compression spring is configured to apply a force to the lock body.

In some examples, a delivery device for a collapsible prosthetic heart valve, the delivery device includes an inner shaft, a distal sheath disposed about a portion of the inner shaft to form a compartment sized to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another, and a handle including a frame having a longitudinal axis, and a deployment actuator operatively connected to the distal sheath, the deployment actuator including a clutch mechanism that rotationally couples the deployment actuator to the distal sheath in a first condition and rotationally decouples the deployment actuator from the distal sheath in a second condition; and/or the deployment actuator includes a wheel shell, and the clutch mechanism includes a clutch plate and a drive nut assembled within the wheel shell; and/or the drive nut includes a plurality of first teeth, each having a sloped portion; and/or the clutch plate includes a plurality of second teeth, complementary to the first teeth, the second teeth being meshed with the plurality of first teeth of the drive nut; and/or the assembly includes a compression spring disposed between the wheel shell and the clutch plate, the compression spring exerting a force pushing the clutch plate against the drive nut.

Although the invention herein has been described with reference to particular embodiments, it is to be understood that these embodiments are merely illustrative of the principles and applications of the present invention. It is therefore to be understood that numerous modifications may be made to the illustrative embodiments and that other arrangements may be devised without departing from the spirit and scope of the present invention as defined by the appended claims.

It will be appreciated that the various dependent claims and the features set forth therein can be combined in different ways than presented in the initial claims. It will also be appreciated that the features described in connection with individual embodiments may be shared with others of the described embodiments.

The invention claimed is:

1. A delivery device for a collapsible prosthetic heart valve, the delivery device comprising:
  - an inner shaft;
  - a distal sheath disposed about a portion of the inner shaft to form a compartment sized to receive the prosthetic heart valve, the inner shaft and the distal sheath being movable relative to one another via a deployment actuator; and
  - a handle including a frame having a longitudinal axis, and the deployment actuator operatively connected to the distal sheath, the deployment actuator including a clutch that rotationally couples the deployment actuator to the distal sheath in a first condition and rotationally decouples the deployment actuator from the distal sheath in a second condition, wherein the clutch comprises a clutch plate rotationally locked to a wheel shell of the deployment actuator in both a first rotational direction and second rotational direction opposite the first rotational direction; and
  - a compression spring disposed between the clutch plate and the wheel shell.
2. The delivery device of claim 1, wherein the clutch includes a drive nut assembled within the wheel shell.

## 17

3. The delivery device of claim 2, wherein the drive nut includes a plurality of first teeth, each having a sloped portion.

4. The delivery device of claim 3, wherein the clutch plate includes a plurality of second teeth, complementary to the first teeth, the second teeth being meshed with the plurality of first teeth of the drive nut.

5. The delivery device of claim 2, further wherein the compression spring exerts a force pushing the clutch plate against the drive nut.

6. The delivery device of claim 5, wherein the force exerted by the compression spring pushes the clutch plate against the drive nut in an axial direction.

7. The delivery device of claim 5, wherein the clutch plate is configured to be disposed circumferentially around a threaded rod.

8. The delivery device of claim 5, wherein the compression spring is concentrically engaged with the drive nut within the wheel shell.

9. The delivery device of claim 2, wherein the clutch plate is engaged with the drive nut assembled within the wheel shell.

10. The delivery device of claim 2, wherein the drive nut includes a plurality of first teeth, each having a perpendicular portion.

11. The delivery device of claim 2, wherein the drive nut is freely rotatable relative to the wheel shell in the second condition.

## 18

12. A clutch in a delivery device for a collapsible prosthetic heart valve, the clutch comprising:

a wheel shell configured to retract a distal sheath of the delivery device;

a clutch plate assembled within the wheel shell and rotationally locked to the wheel shell in both a first rotational direction and second rotational direction opposite the first rotational direction;

a compression spring disposed between the clutch plate and the wheel shell; and

a drive nut positioned adjacent to the clutch plate, wherein the compression spring provides an engagement force that pushes the clutch plate against the drive nut, and wherein the clutch is configured to rotationally couple the wheel shell to the distal sheath in a first condition and to rotationally decouple the wheel shell from the distal sheath in a second condition.

13. The clutch of claim 12, wherein the drive nut has a center opening configured to receive a threaded rod.

14. The clutch of claim 12, wherein the drive nut includes a plurality of first teeth, each having a sloped portion.

15. The clutch of claim 14, wherein the clutch plate includes a plurality of second teeth complementary to the first teeth, the second teeth being meshed with the plurality of first teeth of the drive nut.

\* \* \* \* \*