



US010952850B2

(12) **United States Patent**  
**Hariton et al.**

(10) **Patent No.:** **US 10,952,850 B2**  
(45) **Date of Patent:** **Mar. 23, 2021**

(54) **MINIMALLY-INVASIVE DELIVERY SYSTEMS**

(71) Applicant: **CARDIOVALVE LTD.**, Or Yehuda (IL)

(72) Inventors: **Ilia Hariton**, Zichron Yaakov (IL);  
**Boaz Harari**, Ganey Tikva (IL);  
**Michael Albitov**, Kiryat Ono (IL); **Paul Kaye**, Modiin (IL)

(73) Assignee: **CARDIOVALVE LTD.**, Or Yehuda (IL)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 224 days.

(21) Appl. No.: **16/318,025**

(22) PCT Filed: **Aug. 1, 2017**

(86) PCT No.: **PCT/IL2017/050849**

§ 371 (c)(1),  
(2) Date: **Jan. 15, 2019**

(87) PCT Pub. No.: **WO2018/025263**

PCT Pub. Date: **Feb. 8, 2018**

(65) **Prior Publication Data**

US 2019/0231525 A1 Aug. 1, 2019

(30) **Foreign Application Priority Data**

Aug. 1, 2016 (GB) ..... 1613219.3

(51) **Int. Cl.**

**A61F 2/24** (2006.01)  
**A61F 2/966** (2013.01)  
**A61F 2/958** (2013.01)

(52) **U.S. Cl.**

CPC ..... **A61F 2/2436** (2013.01); **A61F 2/2433** (2013.01); **A61F 2/966** (2013.01); **A61F 2002/9583** (2013.01)

(58) **Field of Classification Search**

CPC ..... **A61F 2/966**; **A61F 2/9661**; **A61F 2/2436**  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,972,494 A 11/1990 White et al.  
5,314,473 A 5/1994 Godin  
(Continued)

FOREIGN PATENT DOCUMENTS

CN 103974674 A 8/2014  
EP 1264582 A2 12/2002  
(Continued)

OTHER PUBLICATIONS

An International Search Report and a Written Opinion both dated Jun. 24, 2020, which issued during the prosecution of Applicant's PCT/IL2019/051398.

(Continued)


*Primary Examiner* — Alexander J Orkin

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **ABSTRACT**

A tool (410) for use with an implant (20) includes a housing (426) and a controller (440). The housing includes a tubular wall (428) that circumscribes a longitudinal axis; is dimensioned to house at least part of the implant; and defines a track (430) that follows a generally-helical path around the longitudinal axis. The controller includes a rod (442) that extends from a proximal part of the tool to the housing; and an actuator (444). The actuator is fixedly coupled to the rod, includes an engaging element (446) that engages the track, and is rotatable with respect to the housing. The controller and the housing mechanically cooperate such that rotation of the actuator with respect to the housing slides the housing longitudinally with respect to the actuator. Other embodiments are also described.

**10 Claims, 16 Drawing Sheets**

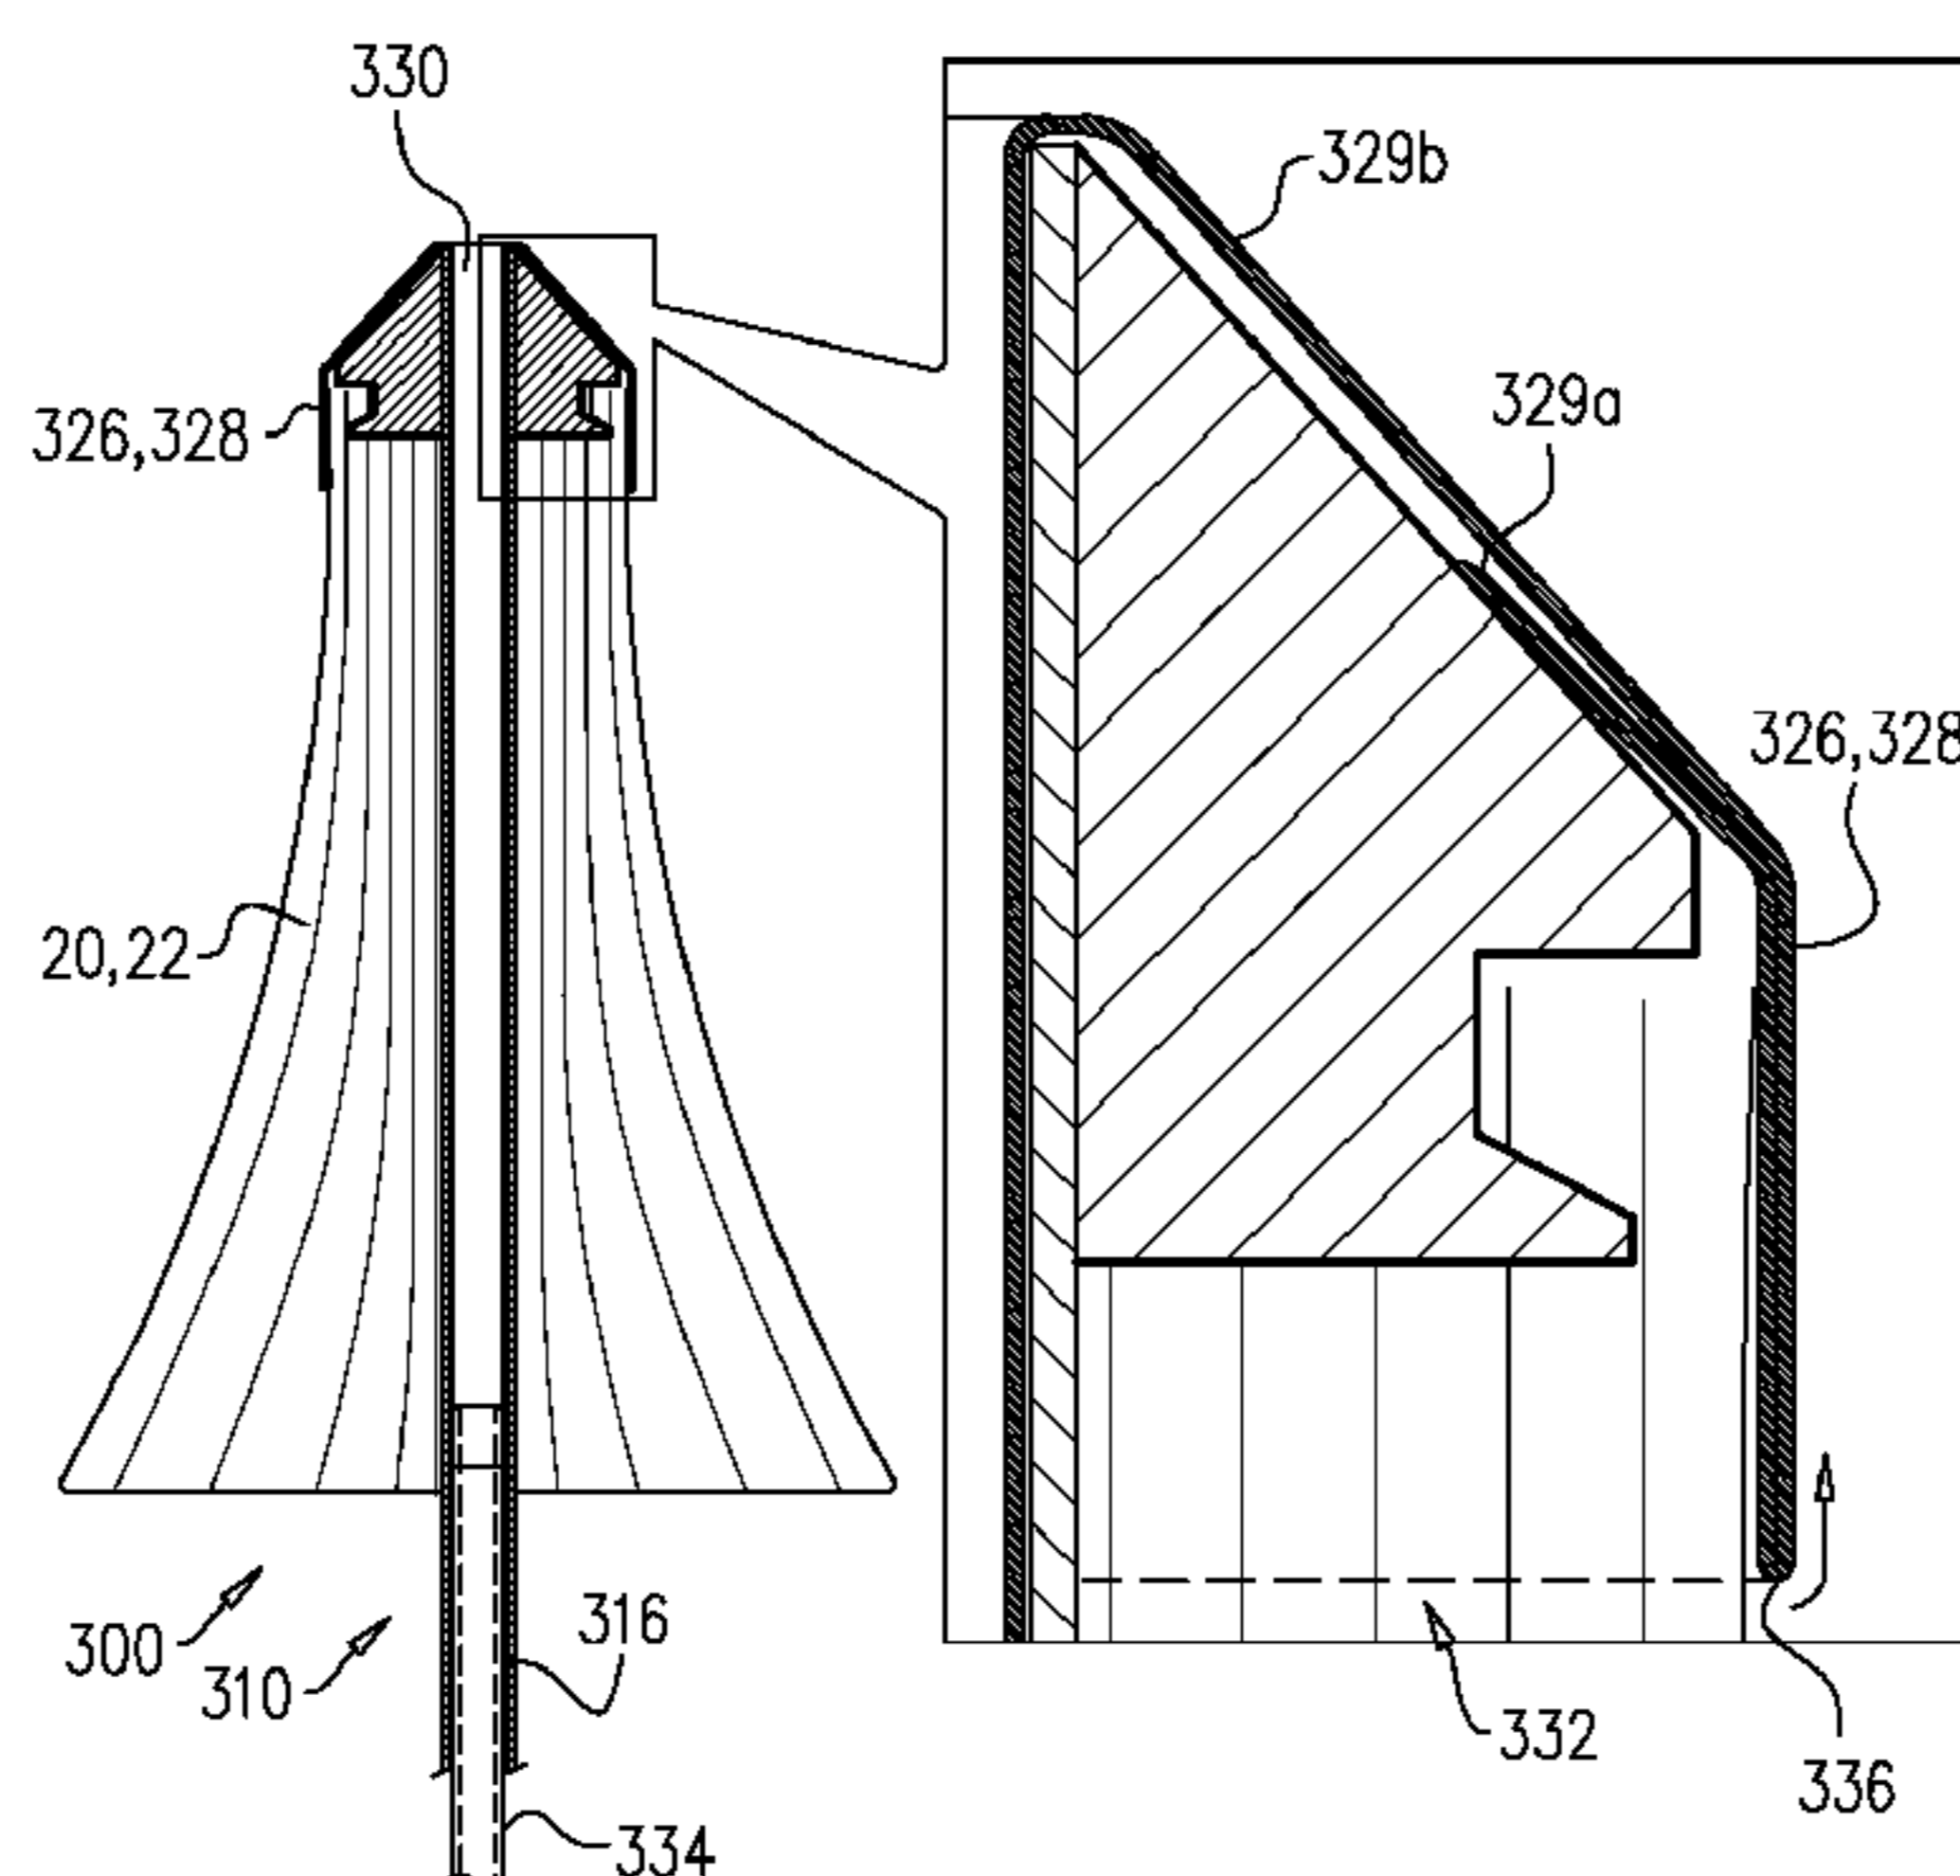



(56)

References Cited

U.S. PATENT DOCUMENTS

5,713,948 A *	2/1998	Uflacker .....	A61F 2/07 606/194	9,987,132 B1	6/2018	Hariton et al.
5,776,140 A	7/1998	Cottone		10,010,414 B2	7/2018	Cooper et al.
5,954,766 A	9/1999	Zadno-Azizi et al.		10,143,552 B2	12/2018	Wallace et al.
5,957,949 A	9/1999	Leonhardt et al.		10,154,903 B2	12/2018	Albitov et al.
6,010,530 A	1/2000	Goicoechea		10,154,906 B2	12/2018	Granada et al.
6,193,686 B1	2/2001	Estrada et al.		10,182,908 B2	1/2019	Tubishevitz et al.
6,264,700 B1	7/2001	Kilcoyne et al.		10,226,341 B2	3/2019	Gross et al.
6,402,780 B2	6/2002	Williamson, IV et al.		10,245,143 B2	4/2019	Gross et al.
6,458,153 B1	10/2002	Bailey et al.		10,258,471 B2	4/2019	Lutter et al.
6,478,807 B1	11/2002	Foreman et al.		10,321,995 B1	6/2019	Christianson et al.
6,491,711 B1	12/2002	Durcan		10,327,895 B2	6/2019	Lozonschi et al.
6,669,724 B2	12/2003	Park et al.		10,376,361 B2	8/2019	Gross et al.
6,764,518 B2	7/2004	Godin		10,531,866 B2	1/2020	Hariton et al.
6,884,257 B1	4/2005	Cox		10,531,872 B2	1/2020	Hacohen et al.
6,951,571 B1	10/2005	Srivastava		10,548,731 B2	2/2020	Lashinski et al.
7,316,716 B2	1/2008	Egan		10,575,948 B2	3/2020	Iamberger et al.
7,442,204 B2	10/2008	Schwammenthal et al.		2001/0002445 A1	5/2001	Vesely
7,585,321 B2	9/2009	Cribier		2002/0032481 A1	3/2002	Gabbay et al.
7,776,080 B2	8/2010	Bei et al.		2002/0151970 A1	10/2002	Garrison et al.
7,837,645 B2	11/2010	Bessler et al.		2002/0177894 A1	11/2002	Acosta et al.
8,029,557 B2	10/2011	Sobino-Serrano et al.		2003/0060875 A1	3/2003	Wittens
8,038,720 B2	10/2011	Wallace et al.		2003/0069635 A1	4/2003	Cartledge et al.
D652,927 S	1/2012	Braido et al.		2004/0133267 A1	7/2004	Lane
D653,341 S	1/2012	Braido et al.		2004/0186558 A1	9/2004	Pavcnik et al.
D660,433 S	5/2012	Braido et al.		2004/0210304 A1	10/2004	Seguin et al.
D660,967 S	5/2012	Braido et al.		2004/0249433 A1	12/2004	Freitag
8,474,460 B2	7/2013	Barrett et al.		2005/0027305 A1	2/2005	Shiu et al.
8,500,821 B2	8/2013	Sobrino-Serrano et al.		2005/0137690 A1	6/2005	Salahieh et al.
8,568,475 B2	10/2013	Nguyen et al.		2005/0149160 A1	7/2005	McFerran
8,579,964 B2	11/2013	Lane et al.		2005/0240200 A1	10/2005	Bergheim
8,591,460 B2	11/2013	Wilson et al.		2005/0251251 A1	11/2005	Cribier
8,628,571 B1	1/2014	Hacohen et al.		2006/0004439 A1	1/2006	Spenser et al.
8,673,020 B2	3/2014	Sobrino-Serrano et al.		2006/0004469 A1	1/2006	Sokel
8,728,155 B2	5/2014	Montorfano et al.		2006/0020327 A1	1/2006	Lashinski et al.
8,784,481 B2	7/2014	Alkhatib et al.		2006/0041189 A1	2/2006	Vancaillie
8,852,272 B2	10/2014	Gross et al.		2006/0052867 A1	3/2006	Revuelta et al.
8,870,948 B1	10/2014	Erzberger et al.		2006/0111773 A1	5/2006	Rittgers et al.
8,870,950 B2	10/2014	Hacohen		2006/0116750 A1	6/2006	Hebert et al.
8,876,800 B2	11/2014	Behan		2006/0155357 A1	7/2006	Melsheimer
8,906,083 B2	12/2014	Obermiller et al.		2006/0241745 A1	10/2006	Solem
8,986,375 B2	3/2015	Garde et al.		2006/0259137 A1	11/2006	Artof et al.
8,998,982 B2	4/2015	Richter et al.		2006/0282150 A1*	12/2006	Olson ..... A61M 25/0136 623/1.11
9,017,399 B2	4/2015	Gross et al.		2007/0027528 A1	2/2007	Agnew
D730,520 S	5/2015	Braido et al.		2007/0027549 A1	2/2007	Godin
D730,521 S	5/2015	Braido et al.		2007/0056346 A1	3/2007	Spenser et al.
9,023,100 B2	5/2015	Quadri et al.		2007/0078510 A1	4/2007	Ryan
D732,666 S	6/2015	Nguyen et al.		2007/0198077 A1	8/2007	Cully et al.
9,050,188 B2	6/2015	Schweich, Jr. et al.		2007/0213810 A1	9/2007	Newhauser et al.
9,095,434 B2	8/2015	Rowe		2007/0219630 A1	9/2007	Chu
9,155,619 B2	10/2015	Liu et al.		2008/0071361 A1	3/2008	Tuval et al.
9,232,995 B2	1/2016	Kovalsky et al.		2008/0082159 A1	4/2008	Tseng et al.
9,241,791 B2	1/2016	Braido et al.		2008/0091261 A1	4/2008	Long et al.
9,241,792 B2	1/2016	Benichou et al.		2008/0132989 A1	6/2008	Snow et al.
9,248,014 B2	2/2016	Lane et al.		2008/0147182 A1	6/2008	Righini et al.
D755,384 S	5/2016	Pesce et al.		2008/0200980 A1	8/2008	Robin et al.
9,326,876 B2	5/2016	Acosta et al.		2008/0269879 A1	10/2008	Sathe et al.
9,387,078 B2	7/2016	Gross et al.		2008/0281411 A1	11/2008	Berrekouw
9,427,303 B2	8/2016	Liddy et al.		2009/0005363 A1	1/2009	Goetz et al.
9,439,757 B2	9/2016	Wallace et al.		2009/0036966 A1	2/2009	O'Connor et al.
9,474,638 B2	10/2016	Robinson et al.		2009/0088836 A1	4/2009	Bishop et al.
9,492,273 B2	11/2016	Wallace et al.		2009/0099554 A1	4/2009	Forster et al.
9,498,314 B2	11/2016	Behan		2009/0125098 A1	5/2009	Chuter
9,510,947 B2	12/2016	Straubinger et al.		2009/0157175 A1	6/2009	Benichou
9,554,899 B2	1/2017	Granada et al.		2009/0240320 A1	9/2009	Tuval et al.
9,561,103 B2	2/2017	Granada et al.		2009/0259306 A1	10/2009	Rowe
9,566,152 B2	2/2017	Schweich, Jr. et al.		2009/0264859 A1	10/2009	Mas
9,662,203 B2	5/2017	Sheahan et al.		2009/0276040 A1	11/2009	Rowe et al.
9,681,952 B2	6/2017	Hacohen et al.		2009/0281619 A1	11/2009	Le et al.
9,717,591 B2	8/2017	Chau et al.		2010/0023120 A1	1/2010	Holeccek et al.
9,743,932 B2	8/2017	Amplatz et al.		2010/0069852 A1	3/2010	Kelley
9,763,657 B2	9/2017	Hacohen et al.		2010/0100167 A1	4/2010	Bortlein et al.
9,763,817 B2	9/2017	Roeder		2010/0161036 A1	6/2010	Pintor et al.
D800,908 S	10/2017	Hariton et al.		2010/0256737 A1	10/2010	Pollock et al.
9,788,941 B2	10/2017	Hacohen		2010/0312333 A1	12/2010	Navia et al.
				2010/0331971 A1	12/2010	Keranen et al.
				2011/0004299 A1	1/2011	Navia et al.
				2011/0021985 A1	1/2011	Spargias
				2011/0029072 A1	2/2011	Gabbay



(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0137397 A1 6/2011 Chau et al.  
 2011/0144742 A1 6/2011 Madrid et al.  
 2011/0208283 A1 8/2011 Rust  
 2011/0213459 A1 9/2011 Garrison et al.  
 2011/0218620 A1 9/2011 Meiri et al.  
 2011/0224785 A1 9/2011 Hacoheh  
 2011/0245911 A1 10/2011 Quill et al.  
 2011/0264196 A1 10/2011 Savage et al.  
 2011/0282439 A1 11/2011 Thill et al.  
 2011/0288632 A1 11/2011 White  
 2011/0295354 A1 12/2011 Bueche et al.  
 2011/0307049 A1\* 12/2011 Kao ..... A61F 2/966  
 623/1.11  
 2011/0313515 A1 12/2011 Quadri et al.  
 2011/0319989 A1 12/2011 Lane et al.  
 2012/0016468 A1 1/2012 Robin et al.  
 2012/0022629 A1 1/2012 Perera et al.  
 2012/0022640 A1 1/2012 Gross et al.  
 2012/0053676 A1 3/2012 Ku et al.  
 2012/0059337 A1 3/2012 Eilat  
 2012/0059458 A1 3/2012 Buchbinder et al.  
 2012/0065464 A1 3/2012 Ellis et al.  
 2012/0078237 A1 3/2012 Wang et al.  
 2012/0078353 A1 3/2012 Quadri et al.  
 2012/0089223 A1 4/2012 Nguyen et al.  
 2012/0101571 A1 4/2012 Thambar et al.  
 2012/0300063 A1 11/2012 Maikrzak et al.  
 2012/0310328 A1 12/2012 Olson et al.  
 2013/0018458 A1 1/2013 Yohanan et al.  
 2013/0035759 A1 2/2013 Gross et al.  
 2013/0079872 A1 3/2013 Gallagher  
 2013/0150956 A1 6/2013 Yohanan et al.  
 2013/0190861 A1 7/2013 Chau et al.  
 2013/0231735 A1 9/2013 Deem et al.  
 2013/0261738 A1 10/2013 Clague et al.  
 2013/0289711 A1 10/2013 Liddy et al.  
 2013/0304200 A1 11/2013 McLean et al.  
 2013/0323316 A1 12/2013 Vogel et al.  
 2014/0000112 A1 1/2014 Braido et al.  
 2014/0005778 A1 1/2014 Buchbinder et al.  
 2014/0018915 A1 1/2014 Biadillah et al.  
 2014/0121749 A1 5/2014 Roeder  
 2014/0142688 A1 5/2014 Duffy et al.  
 2014/0172077 A1 6/2014 Bruchman et al.  
 2014/0172082 A1 6/2014 Bruchman et al.  
 2014/0194981 A1 7/2014 Menk et al.  
 2014/0207231 A1 7/2014 Hacoheh et al.  
 2014/0222136 A1 8/2014 Geist et al.  
 2014/0222142 A1 8/2014 Kovalsky et al.  
 2014/0236287 A1 8/2014 Clague et al.  
 2014/0236289 A1 8/2014 Alkhatib  
 2014/0249622 A1 9/2014 Carmi et al.  
 2014/0257461 A1 9/2014 Robinson et al.  
 2014/0257467 A1 9/2014 Lane et al.  
 2014/0277409 A1 9/2014 Börtlein et al.  
 2014/0277411 A1 9/2014 Börtlein et al.  
 2014/0277418 A1 9/2014 Miller  
 2014/0336744 A1 11/2014 Tani et al.  
 2014/0343670 A1 11/2014 Bakis et al.  
 2015/0018944 A1 1/2015 O'Connell et al.  
 2015/0119970 A1 4/2015 Nakayama et al.  
 2015/0142100 A1 5/2015 Morriss et al.  
 2015/0148894 A1 5/2015 Damm et al.  
 2015/0157458 A1 6/2015 Thambar et al.  
 2015/0173896 A1 6/2015 Richter et al.  
 2015/0173897 A1 6/2015 Raanani et al.  
 2015/0238313 A1 8/2015 Spence et al.  
 2015/0245934 A1 9/2015 Lombardi et al.  
 2015/0272730 A1 10/2015 Melnick et al.  
 2015/0272734 A1 10/2015 Sheps et al.  
 2015/0282964 A1 10/2015 Beard et al.  
 2015/0320556 A1 11/2015 Levi et al.  
 2015/0327994 A1 11/2015 Morriss et al.  
 2015/0335429 A1 11/2015 Morriss et al.  
 2015/0342736 A1 12/2015 Rabito et al.

2015/0351903 A1 12/2015 Morriss et al.  
 2015/0351904 A1 12/2015 Cooper et al.  
 2015/0359629 A1 12/2015 Ganesan et al.  
 2016/0030169 A1 2/2016 Shahriari  
 2016/0030171 A1 2/2016 Quijano et al.  
 2016/0113766 A1 4/2016 Ganesan et al.  
 2016/0113768 A1 4/2016 Ganesan et al.  
 2016/0125160 A1 5/2016 Heneghan et al.  
 2016/0220367 A1 8/2016 Barrett  
 2016/0228247 A1 8/2016 Maimon et al.  
 2016/0270911 A1 9/2016 Ganesan et al.  
 2016/0317301 A1 11/2016 Quadri et al.  
 2016/0317305 A1 11/2016 Pelled et al.  
 2016/0324635 A1 11/2016 Vidlund et al.  
 2016/0331526 A1 11/2016 Schweich, Jr. et al.  
 2016/0331527 A1 11/2016 Vidlund et al.  
 2016/0374801 A1 12/2016 Jimenez et al.  
 2016/0374802 A1 12/2016 Levi et al.  
 2017/0042678 A1 2/2017 Ganesan et al.  
 2017/0056166 A1 3/2017 Ratz et al.  
 2017/0056171 A1 3/2017 Cooper et al.  
 2017/0128205 A1 5/2017 Tamir et al.  
 2017/0135816 A1 5/2017 Lashinski et al.  
 2017/0189174 A1 7/2017 Braido et al.  
 2017/0196688 A1 7/2017 Christianson et al.  
 2017/0196692 A1 7/2017 Kirk et al.  
 2017/0209264 A1 7/2017 Chau et al.  
 2017/0216026 A1 8/2017 Quill et al.  
 2017/0231759 A1 8/2017 Geist et al.  
 2017/0231760 A1 8/2017 Lane et al.  
 2017/0333187 A1 11/2017 Hariton et al.  
 2018/0000580 A1 1/2018 Wallace et al.  
 2018/0021129 A1 1/2018 Peterson et al.  
 2018/0049873 A1 2/2018 Manash et al.  
 2018/0055628 A1 3/2018 Patel et al.  
 2018/0055630 A1 3/2018 Patel et al.  
 2018/0125644 A1 5/2018 Conklin  
 2018/0153689 A1 6/2018 Maimon et al.  
 2018/0153696 A1 6/2018 Albitov et al.  
 2018/0177593 A1 6/2018 Hariton et al.  
 2018/0177594 A1 6/2018 Patel et al.  
 2018/0185148 A1 7/2018 Hariton et al.  
 2018/0206983 A1 7/2018 Noe et al.  
 2018/0250126 A1 9/2018 O'connor et al.  
 2018/0296336 A1 10/2018 Cooper et al.  
 2018/0296341 A1 10/2018 Noe et al.  
 2018/0344457 A1 12/2018 Gross et al.  
 2018/0353294 A1 12/2018 Calomeni et al.  
 2019/0053896 A1 2/2019 Adamek-bowers et al.  
 2019/0060060 A1 2/2019 Chau et al.  
 2019/0060068 A1 2/2019 Cope et al.  
 2019/0060070 A1 2/2019 Groothuis et al.  
 2019/0069997 A1 3/2019 Ratz et al.  
 2019/0105153 A1 4/2019 Barash et al.  
 2019/0117391 A1 4/2019 Humair  
 2019/0167423 A1 6/2019 Hariton et al.  
 2019/0175339 A1 6/2019 Vidlund  
 2019/0183639 A1 6/2019 Moore  
 2019/0216602 A1 7/2019 Lozonschi  
 2019/0350701 A1 11/2019 Adamek-bowers et al.  
 2019/0365530 A1 12/2019 Hoang et al.  
 2019/0388218 A1 12/2019 Vidlund et al.  
 2019/0388220 A1 12/2019 Vidlund et al.  
 2020/0000579 A1 1/2020 Manash et al.  
 2020/0015964 A1 1/2020 Noe et al.  
 2020/0060818 A1 2/2020 Geist et al.

FOREIGN PATENT DOCUMENTS

EP 1768630 B1 4/2007  
 JP 53-152790 12/1978  
 KR 2001-0046894 A 6/2001  
 WO 98/43557 A1 10/1998  
 WO 01/82832 A2 11/2001  
 WO 2005/107650 A2 11/2005  
 WO 2006/007401 A2 1/2006  
 WO 2007/059252 A1 5/2007  
 WO 2008/031103 A2 3/2008  
 WO 2008/070797 A2 6/2008



(56)

## References Cited

## FOREIGN PATENT DOCUMENTS

WO	2009/091509	A1	7/2009
WO	2010/006627	A2	1/2010
WO	2010/037141	A1	4/2010
WO	2010/057262	A1	5/2010
WO	2016/125160	A1	8/2010
WO	2010/121076	A2	10/2010
WO	2011/025972	A2	3/2011
WO	2012/024428	A2	2/2012
WO	2012036740	A2	3/2012
WO	2012/048035	A2	4/2012
WO	2013/021374	A2	2/2013
WO	2013/021375	A2	2/2013
WO	2013/059747	A1	4/2013
WO	2013/072496		5/2013
WO	2013/078497	A1	6/2013
WO	2013/175468		11/2013
WO	2014/076696	A1	5/2014
WO	2014/115149	A2	7/2014
WO	2014/164364	A1	10/2014
WO	2014/194178	A1	12/2014
WO	2016/016899	A1	2/2016
WO	2017/223486	A1	12/2017
WO	2018/025260	A2	2/2018
WO	2018/025263	A2	2/2018
WO	2018/029680	A1	2/2018
WO	2018/039631	A1	3/2018
WO	2018/106837	A1	6/2018
WO	2018/112429	A1	6/2018
WO	2018/118717	A1	6/2018
WO	2018/131042	A1	7/2018
WO	2018/131043	A1	7/2018
WO	2019/026059	A1	2/2019
WO	2019/030753	A1	2/2019
WO	2019/077595	A1	4/2019
WO	2019/116369	A1	6/2019
WO	2019/138400	A1	7/2019
WO	2019/195860		10/2019
WO	2019/202579	A1	10/2019
WO	2020/058972	A1	3/2020

## OTHER PUBLICATIONS

An Office Action dated Aug. 7, 2020, which issued during the prosecution of U.S. Appl. No. 15/668,659.

An Office Action dated Jul. 14, 2020, which issued during the prosecution of U.S. Appl. No. 16/324,339.

An Office Action dated Jul. 29, 2020, which issued during the prosecution of U.S. Appl. No. 16/269,328.

An Office Action summarized English translation and Search Report dated Jul. 3, 2020, which issued during the prosecution of Chinese Patent Application No. 201780061210.3.

Notice of Allowance dated Aug. 26, 2020, which issued during the prosecution of U.S. Appl. No. 16/269,328.

Notice of Allowance dated Aug. 28, 2020, which issued during the prosecution of U.S. Appl. No. 16/324,339.

Notice of Allowance dated Jul. 29, 2020, which issued during the prosecution of U.S. Appl. No. 16/132,937.

Notice of Allowance dated May 7, 2020, which issued during the prosecution of U.S. Appl. No. 16/637,166.

Notice of Allowance dated Sep. 10, 2020, which issued during the prosecution of U.S. Appl. No. 15/600,190.

Serruys, P. W., Piazza, N., Cribier, A., Webb, J., Laborde, J. C., & de Jaegere, P. (Eds.). (2009). Transcatheter aortic valve implantation: tips and tricks to avoid failure. CRC Press.—Screenshots from Google Books downloaded from: [https://books.google.co.il/books?id=FLzLBQAAQBAJ&Ipg=PA198&ots=sogWrDH-y\\_&dq=%20%22Edwards%20SAPIEN%22&lr&pg=PA20#v=onepage&q=%22Edwards%20SAPIEN%22&f=false](https://books.google.co.il/books?id=FLzLBQAAQBAJ&Ipg=PA198&ots=sogWrDH-y_&dq=%20%22Edwards%20SAPIEN%22&lr&pg=PA20#v=onepage&q=%22Edwards%20SAPIEN%22&f=false) ; Downloaded on Jun. 18, 2020.

Sündermann, Simon H., et al. "Feasibility of the Engager™ aortic transcatheter valve system using a flexible over-the-wire design." *European Journal of Cardio-Thoracic Surgery* 42.4 (2012): e48-e52.

Symetis S.A.: "ACURATE neo™ Aortic Bioprosthesis for Implantation using the ACURATE neo™ TA Transapical Delivery System in Patients with Severe Aortic Stenosis," Clinical Investigation Plan, Protocol No. 2015-01, Vs. No. 2, 2015:1-76.

Tchetche, D. and Nicolas M. Van Mieghem: "New-generation TAVI devices: description and specifications" *EuroIntervention*, 2014, No. 10:U90-U100.

An Office Action dated May 8, 2018, which issued during the prosecution of U.S. Appl. No. 15/902,403.

An International Preliminary Report on Patentability dated Feb. 5, 2019, which issued during the prosecution of Applicant's PCT/IL2017/050849.

European Search Report dated Sep. 26, 2018 which issued during the prosecution of Applicant's European App No. 18188784.7.

An Invitation to pay additional fees dated Oct. 11, 2018, which issued during the prosecution of Applicant's PCT/IL2018/050725.

An Office Action together with the English translation dated Nov. 5, 2018 which issued during the prosecution of Chinese Patent Application No. 201680008328.5.

Notice of Allowance dated Sep. 25, 2018, which issued during the prosecution of U.S. Appl. No. 15/188,507.

An International Search Report and a Written Opinion both dated Mar. 27, 2018, which issued during the prosecution of Applicant's PCT/IL2017/050849.

Notice of Allowance dated Oct. 5, 2018, which issued during the prosecution of U.S. Appl. No. 15/886,517.

An Office Action dated Dec. 4, 2018, which issued during the prosecution of U.S. Appl. No. 16/045,059.

An Office Action dated Feb. 5, 2019, which issued during the prosecution of U.S. Appl. No. 15/899,858.

An Office Action dated May 11, 2018, which issued during the prosecution of U.S. Appl. No. 15/899,858.

USPTO NFOA dated Oct. 23, 2017 in connection with U.S. Appl. No. 14/763,004.

USPTO FOA dated Jan. 17, 2018 in connection with U.S. Appl. No. 14/763,004.

USPTO NFOA dated Feb. 7, 2018 in connection with U.S. Appl. No. 15/197,069.

USPTO NFOA dated Dec. 7, 2017 in connection with U.S. Appl. No. 15/213,791.

Interview Summary dated Feb. 8, 2018 in connection with U.S. Appl. No. 15/213,791.

USPTO NFOA dated Jan. 5, 2018 in connection with U.S. Appl. No. 15/541,783.

USPTO NFOA dated Feb. 2, 2018 in connection with U.S. Appl. No. 15/329,920.

Invitation to pay additional fees dated Jan. 2, 2018; PCT/IL2017/050849.

UK Office Action dated Feb. 8, 2017; Appln. No. 1613219.3.

An Office Action dated Jun. 6, 2018, which issued during the prosecution of UK Patent Application No. 1720803.4.

An Office Action dated Jun. 18, 2018, which issued during the prosecution of UK Patent Application No. 1800399.6.

International Search Report and Written Opinion dated Jun. 20, 2018 PCT/IL2018/050024.

USPTO AA dated Apr. 2, 2018 in connection with U.S. Appl. No. 14/763,004.

USPTO NFOA dated Jun. 28, 2018 in connection with U.S. Appl. No. 29/635,658.

USPTO NFOA dated Jun. 28, 2018 in connection with U.S. Appl. No. 29/635,661.

USPTO NFOA dated Jul. 26, 2018 in connection with U.S. Appl. No. 15/872,501.

USPTO NFOA dated Aug. 9, 2018 in connection with U.S. Appl. No. 15/899,858.

USPTO NOA mailed Apr. 20, 2018 in connection with U.S. Appl. No. 15/878,206.

USPTO RR dated May 4, 2018 in connection with U.S. Appl. No. 15/872,501.

USPTO NFOA dated Apr. 20, 2018 in connection with U.S. Appl. No. 15/886,517.

USPTO NFOA dated Aug. 9, 2018 in connection with U.S. Appl. No. 15/902,403.



(56)

**References Cited**

## OTHER PUBLICATIONS

An Office Action dated May 16, 2019, which issued during the prosecution of U.S. Appl. No. 15/433,547.  
 An Office Action dated Jun. 25, 2019, which issued during the prosecution of U.S. Appl. No. 15/329,920.  
 An Office Action dated Jun. 19, 2019, which issued during the prosecution of U.S. Appl. No. 15/682,789.  
 An Office Action dated Sep. 13, 2019, which issued during the prosecution of U.S. Appl. No. 16/460,313.  
 An Office Action dated Nov. 26, 2019, which issued during the prosecution of U.S. Appl. No. 16/532,945.  
 An Office Action dated Oct. 4, 2019, which issued during the prosecution of U.S. Appl. No. 16/183,140.  
 An Office Action dated Jun. 14, 2019, which issued during the prosecution of U.S. Appl. No. 15/703,385.  
 An Office Action dated Aug. 1, 2019, which issued during the prosecution of U.S. Appl. No. 15/668,559.  
 An Office Action dated Aug. 16, 2019, which issued during the prosecution of U.S. Appl. No. 15/668,659.  
 An Office Action dated Jun. 13, 2019, which issued during the prosecution of U.S. Appl. No. 16/388,038.  
 An Office Action dated Nov. 1, 2019 which issued during the prosecution of U.S. Appl. No. 15/872,501.  
 An Office Action dated Jan. 6, 2020, which issued during the prosecution of U.S. Appl. No. 16/660,231.  
 An Office Action dated Dec. 31, 2019, which issued during the prosecution of U.S. Appl. No. 16/183,140.  
 An Office Action dated Jan. 14, 2020, which issued during the prosecution of U.S. Appl. No. 16/284,331.  
 Notice of Allowance dated Jan. 13, 2020, which issued during the prosecution of U.S. Appl. No. 15/956,956.  
 European Search Report dated Mar. 5, 2020 which issued during the prosecution of Applicant's European App No. 17752184.6.  
 European Search Report dated Mar. 4, 2020 which issued during the prosecution of Applicant's European App No. 16706913.7.  
 Notice of Allowance dated Mar. 12, 2020, which issued during the prosecution of U.S. Appl. No. 16/460,313.

An Office Action dated Jan. 9, 2020, which issued during the prosecution of U.S. Appl. No. 15/600,190.  
 An Office Action dated Jan. 3, 2020, which issued during the prosecution of U.S. Appl. No. 16/678,355.  
 An Office Action dated Feb. 6, 2020, which issued during the prosecution of U.S. Appl. No. 15/668,659.  
 An International Search Report and Written Opinion both dated Nov. 9, 2018, which issued during the prosecution of Applicant's PCT/IL2018/050869.  
 An International Search Report and a Written Opinion both dated May 13, 2019, which issued during the prosecution of Applicant's PCT/IL2018/051350.  
 An International Search Report and a Written Opinion both dated Apr. 25, 2019, which issued during the prosecution of Applicant's PCT/IL2019/050142.  
 An International Search Report and a Written Opinion both dated Jan. 25, 2019, which issued during the prosecution of Applicant's PCT/IL2018/051122.  
 An International Search Report and a Written Opinion both dated Dec. 5, 2018, which issued during the prosecution of Applicant's PCT/IL2018/050725.  
 An International Preliminary Report on Patentability dated Feb. 12, 2019, which issued during the prosecution of Applicant's PCT/IL2017/050873.  
 An Office Action dated Mar. 25, 2019, which issued during the prosecution of European Patent Application No. 14710060.6.  
 An Office Action dated May 1, 2019, which issued during the prosecution U.S. Appl. No. 15/691,032.  
 An Office Action dated Oct. 25, 2018, which issued during the prosecution of U.S. Appl. No. 14/763,004.  
 An Office Action dated Mar. 4, 2019, which issued during the prosecution of U.S. Appl. No. 14/763,004.  
 An Office Action dated Jan. 9, 2019, which issued during the prosecution of U.S. Appl. No. 15/329,920.  
 An Office Action dated Jan. 30, 2019, which issued during the prosecution of U.S. Appl. No. 15/872,501.  
 An Office Action dated May 23, 2019, which issued during the prosecution of U.S. Appl. No. 15/668,659.

\* cited by examiner



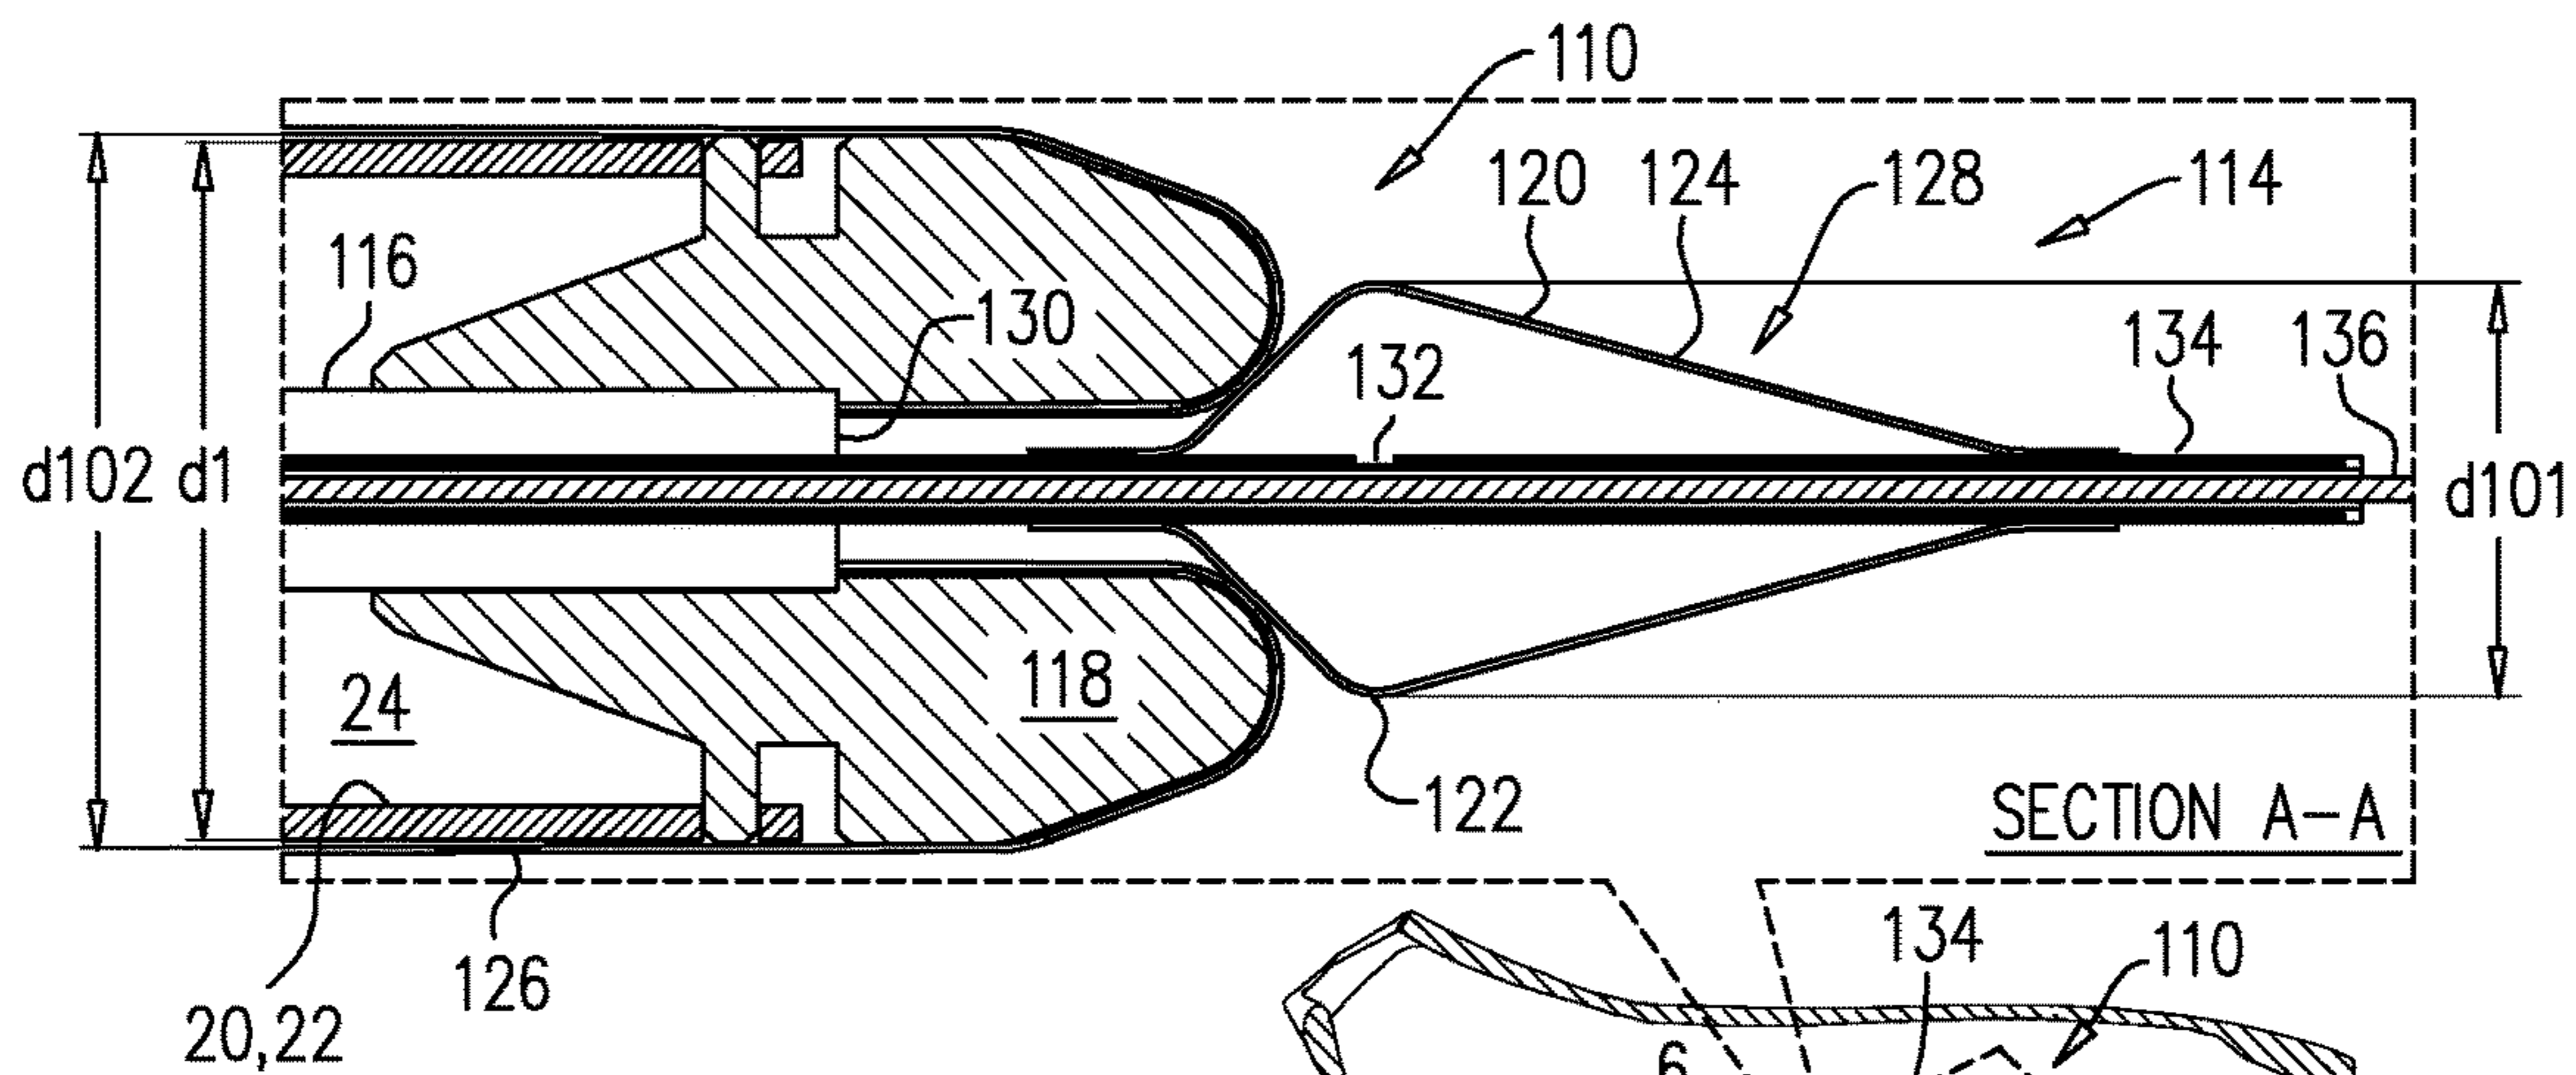


FIG. 1A

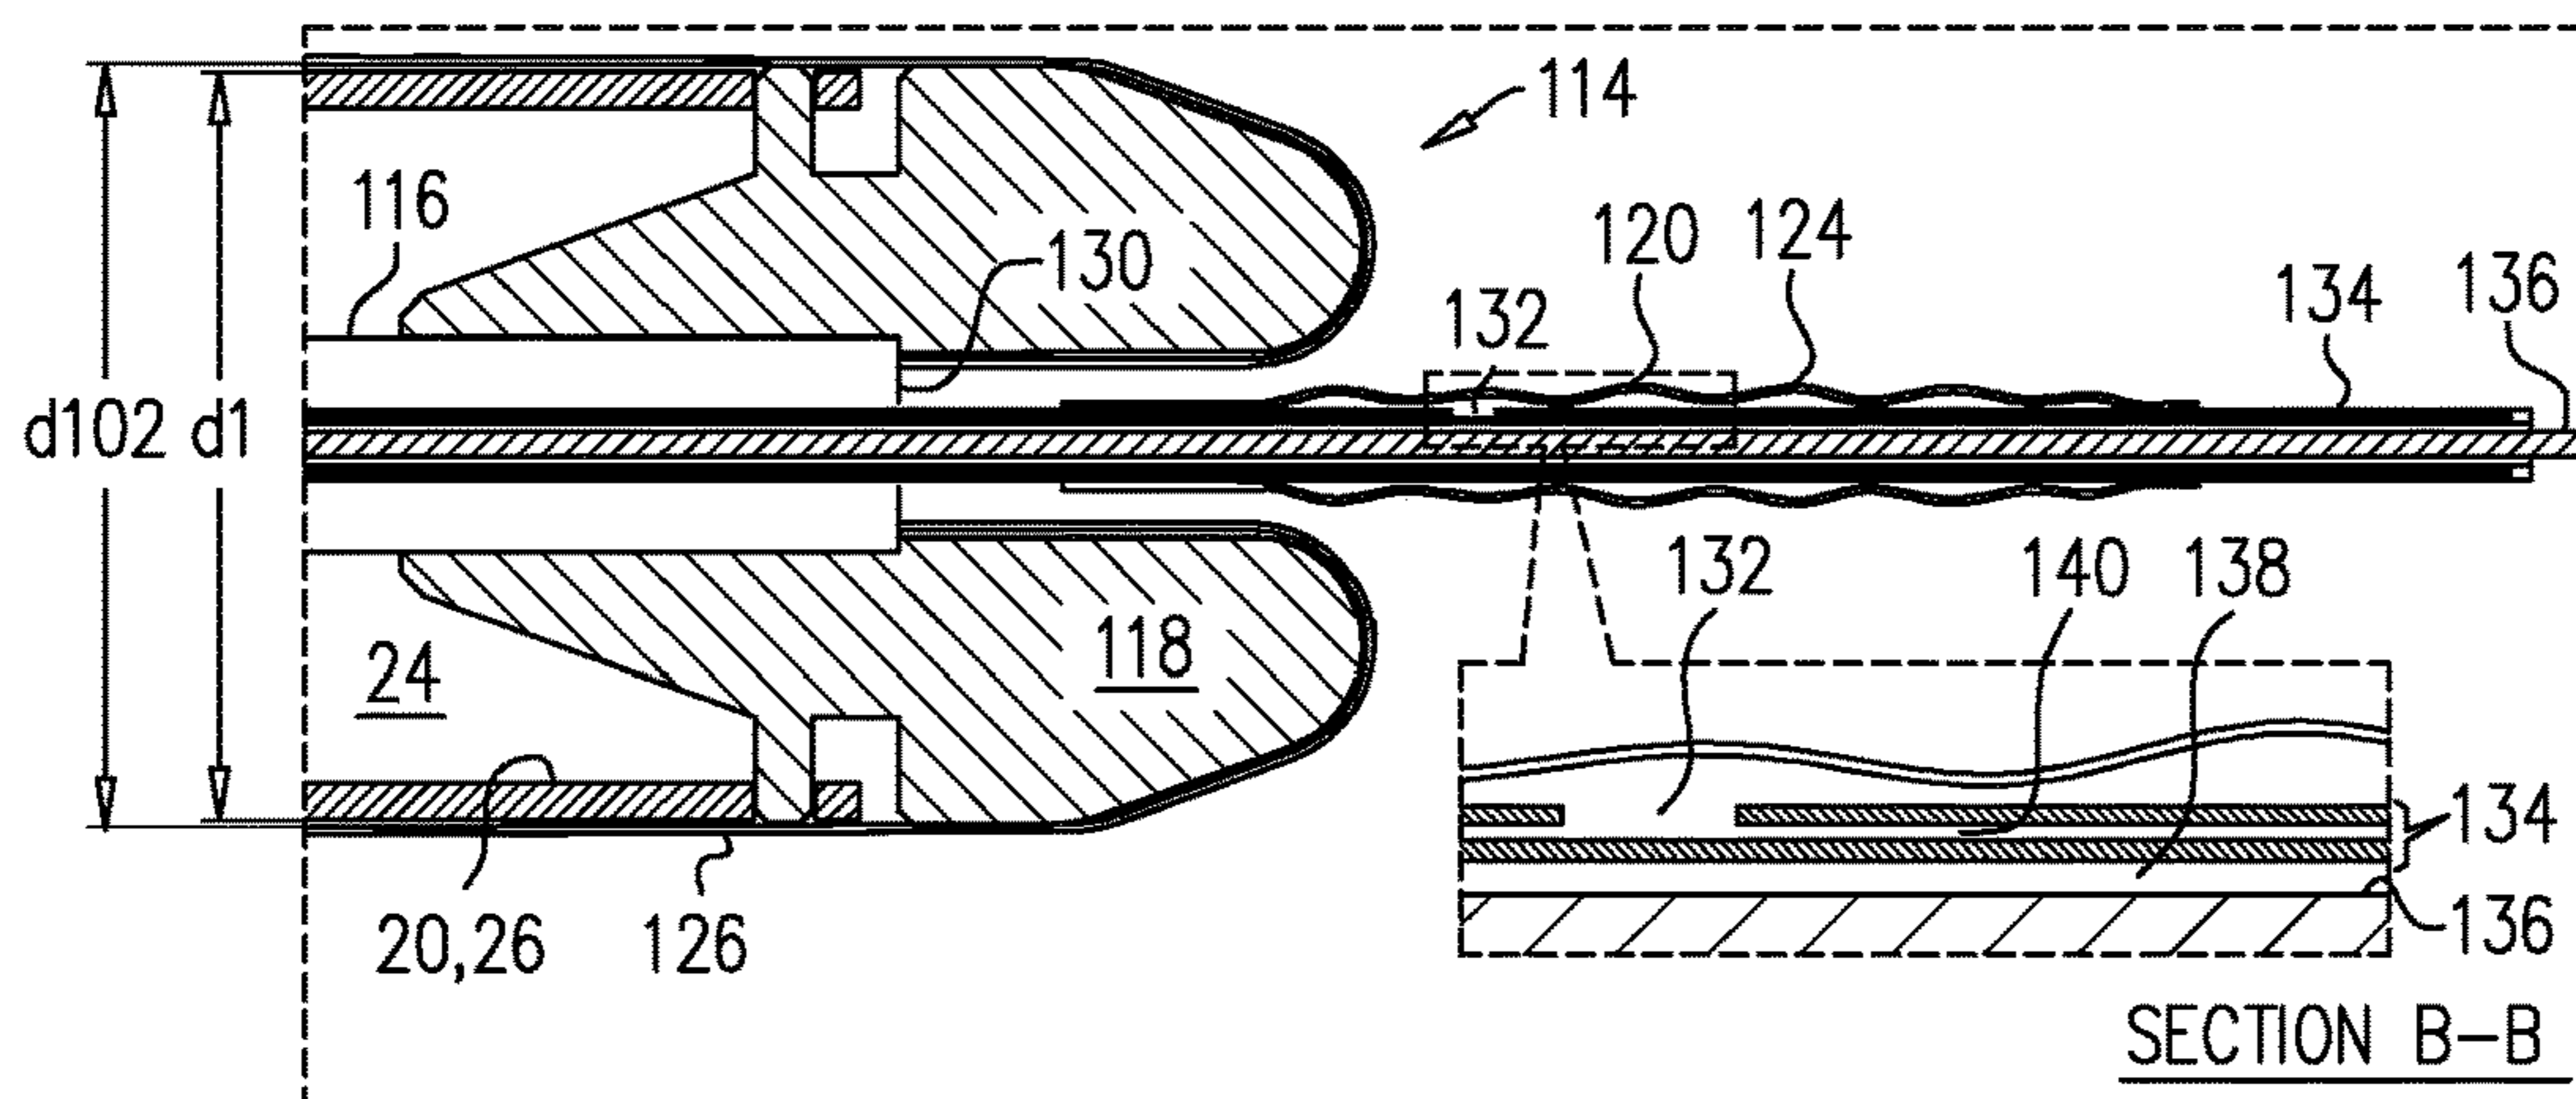
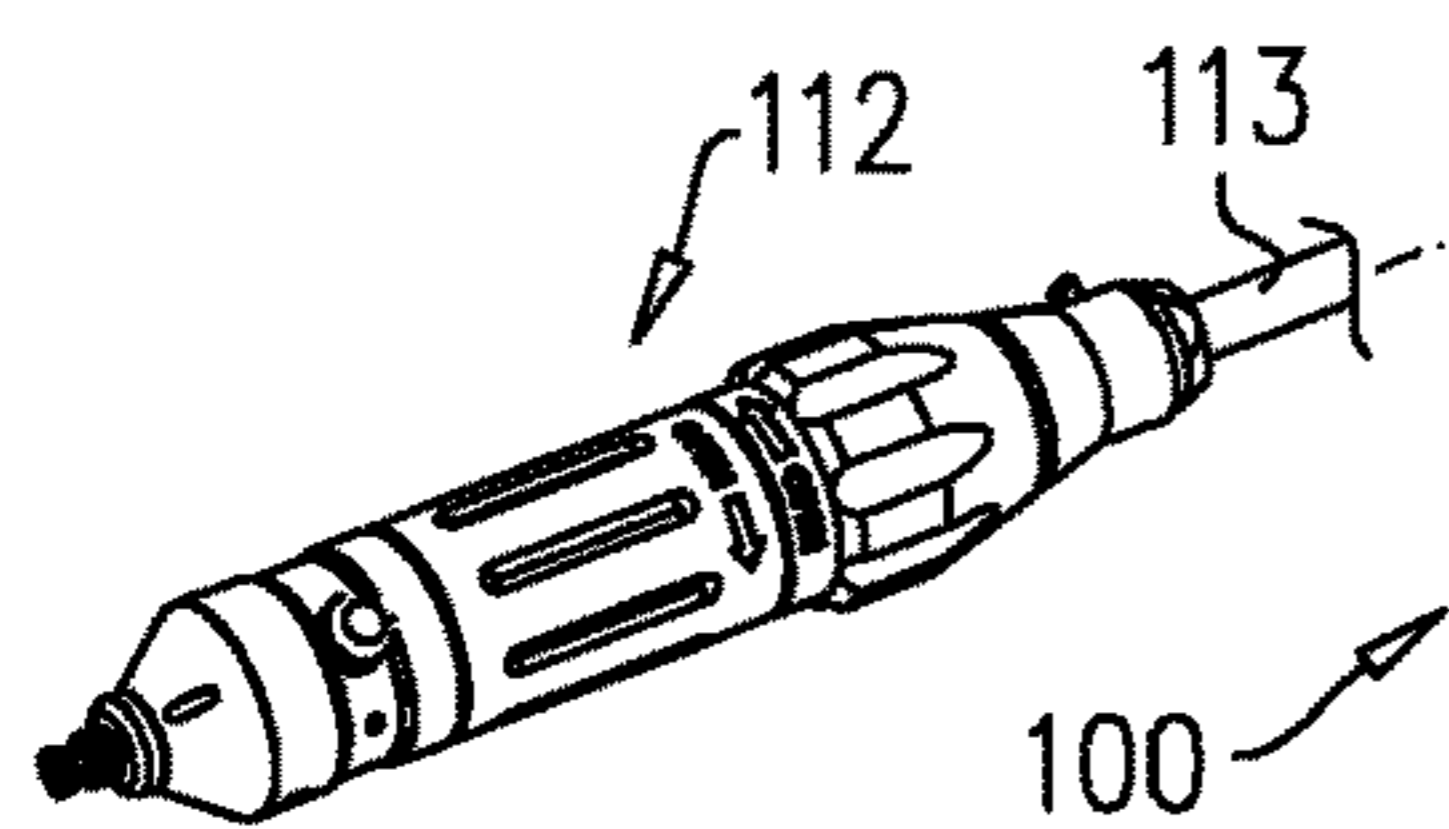
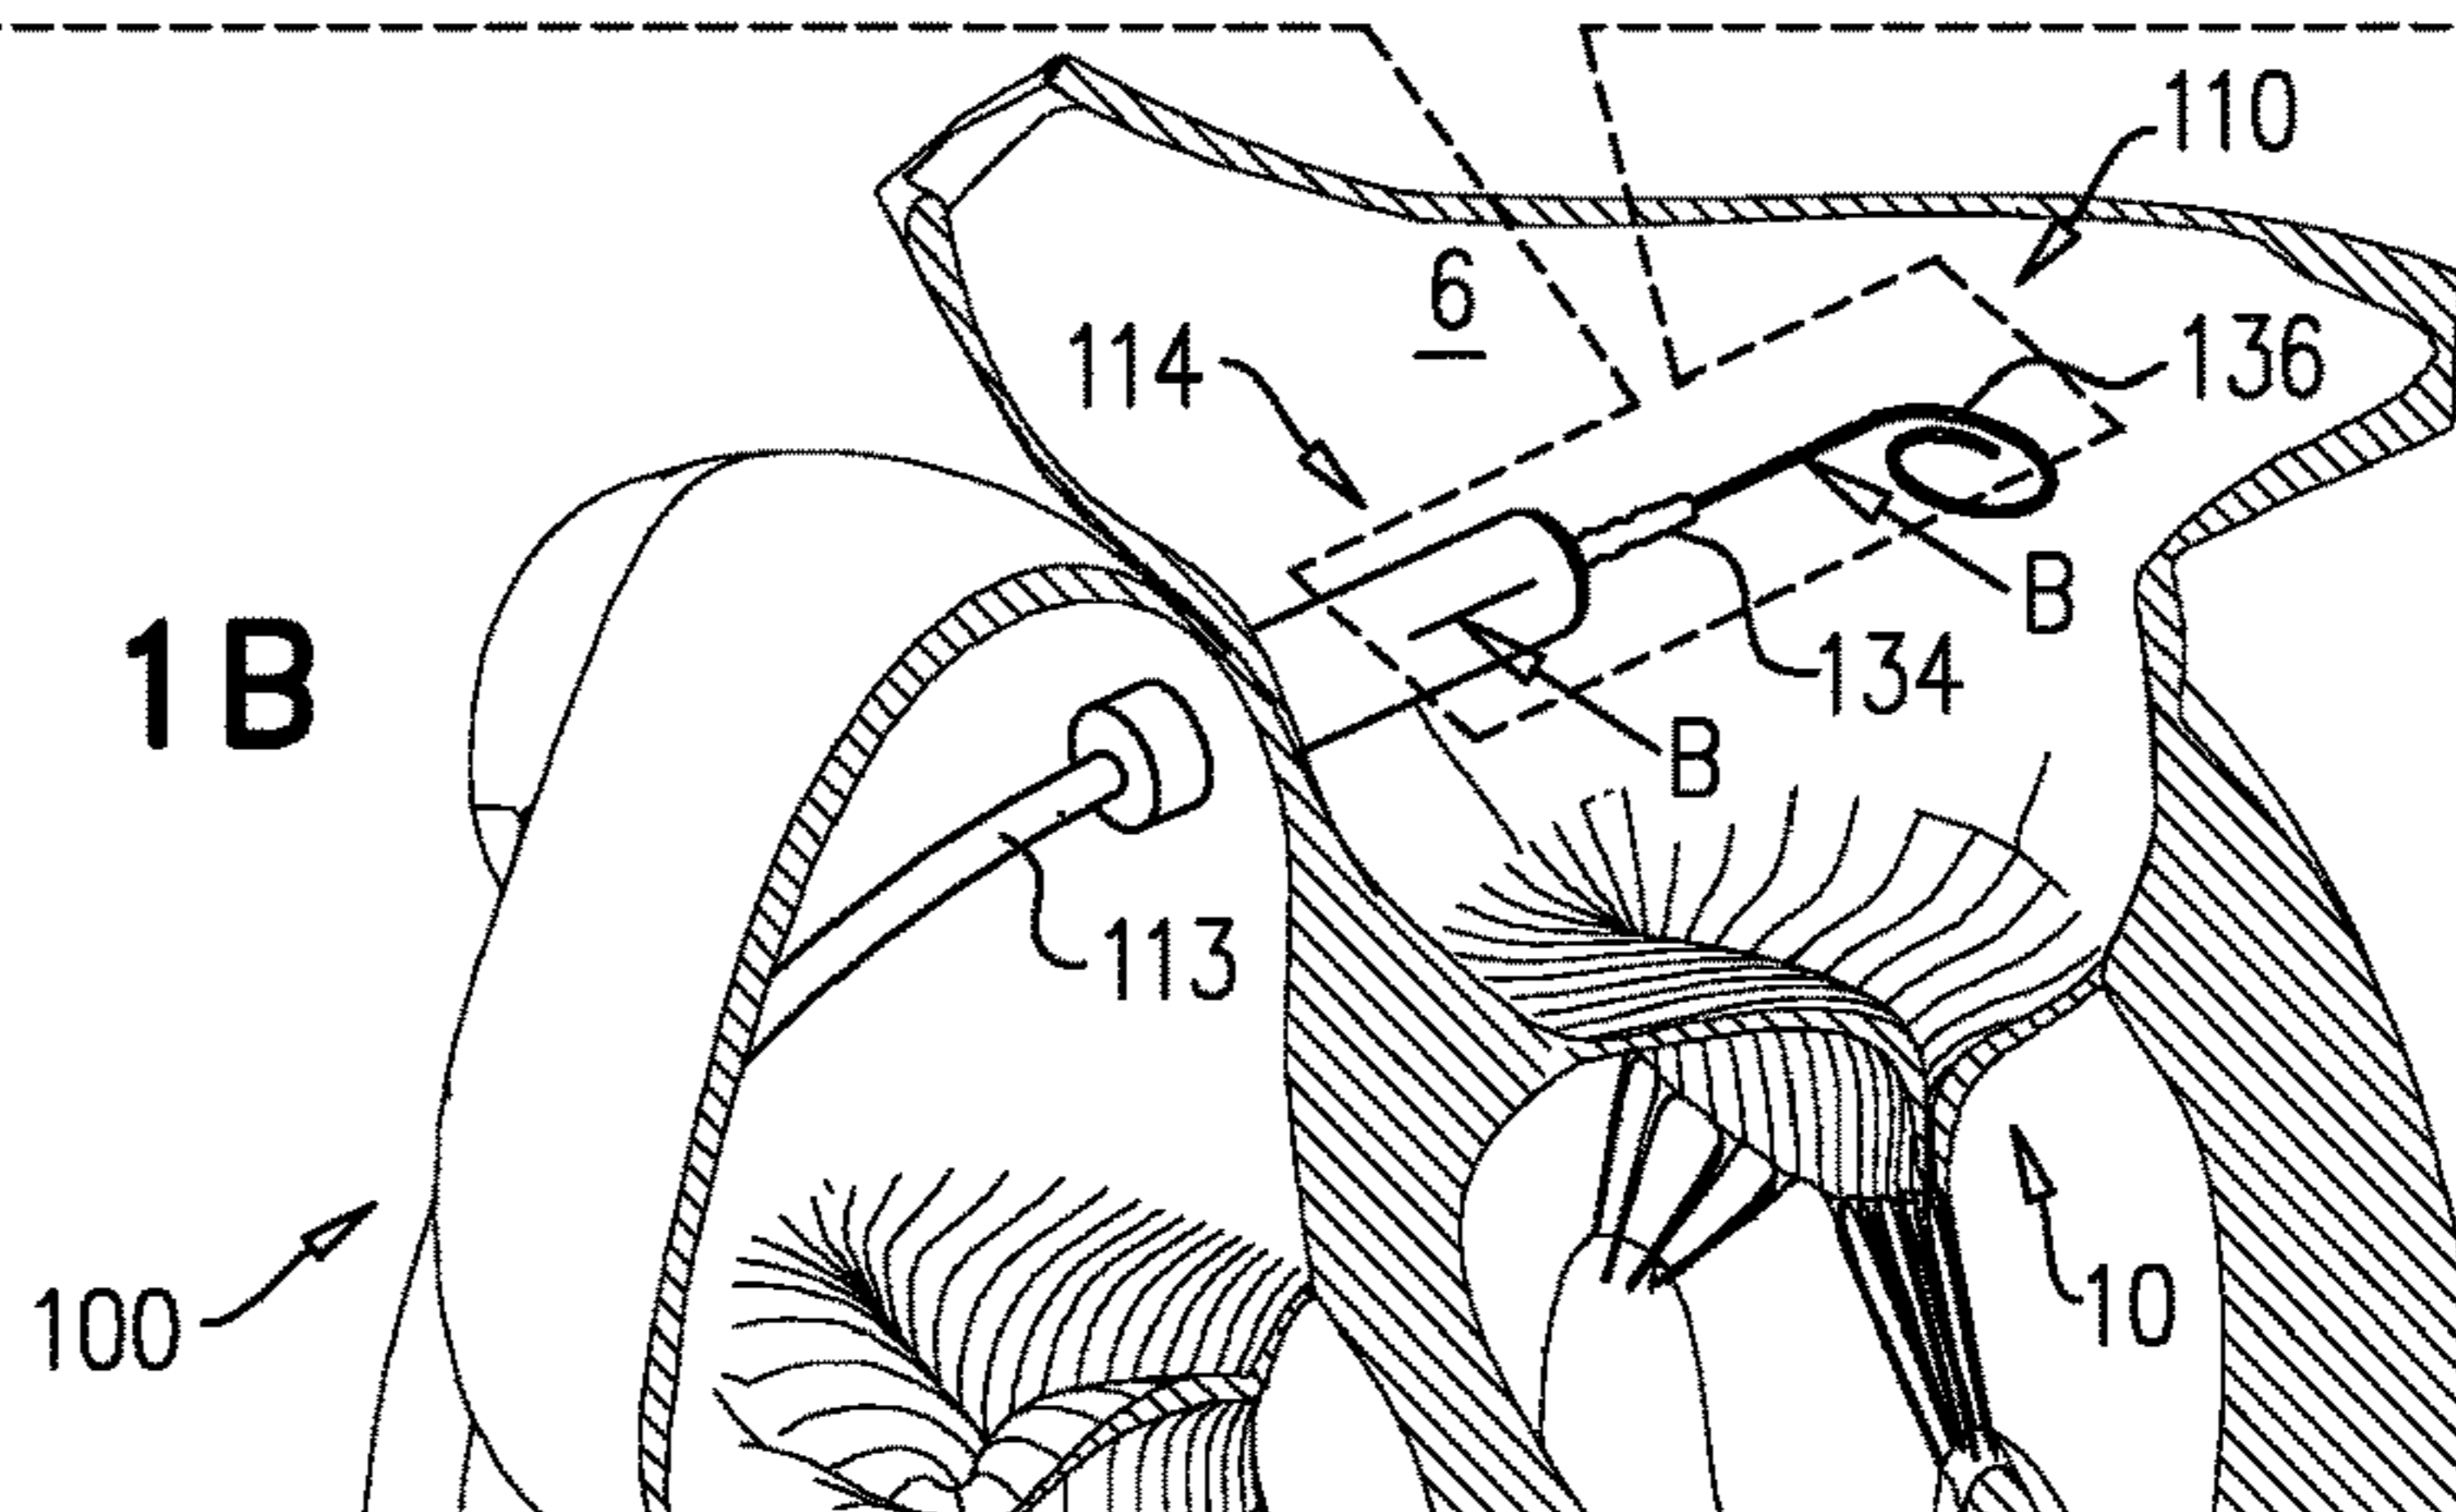


FIG. 1B



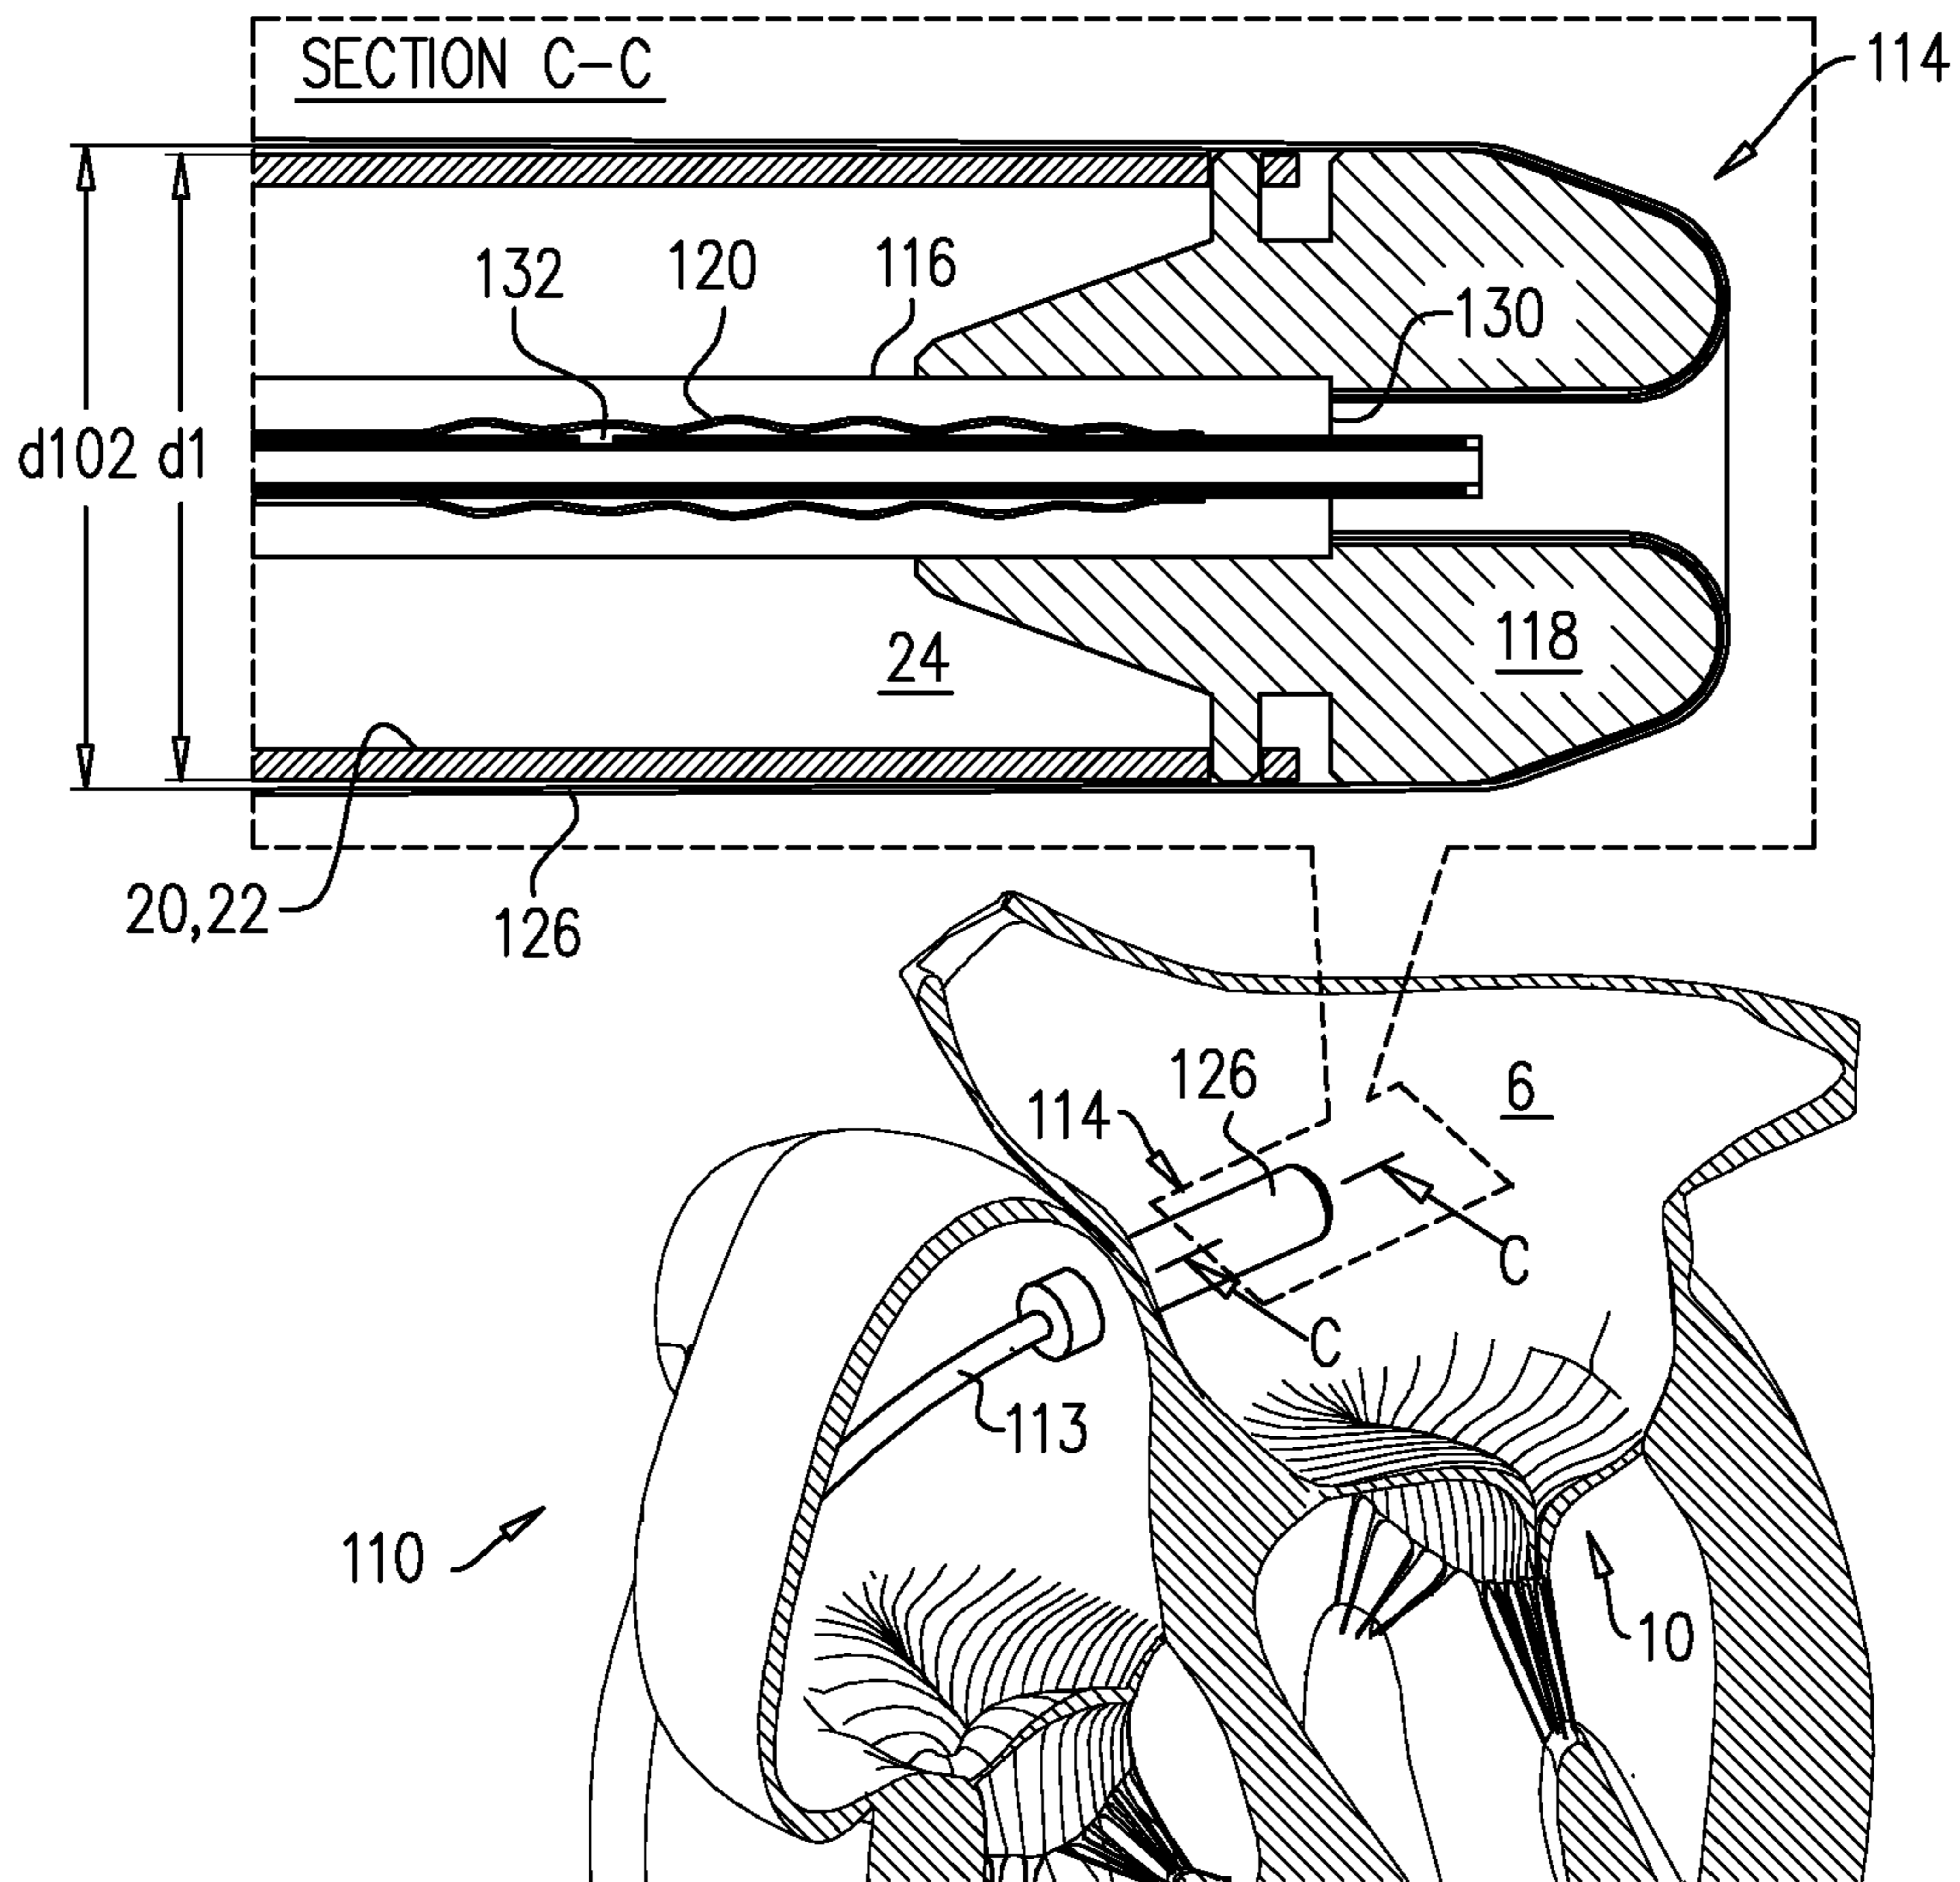
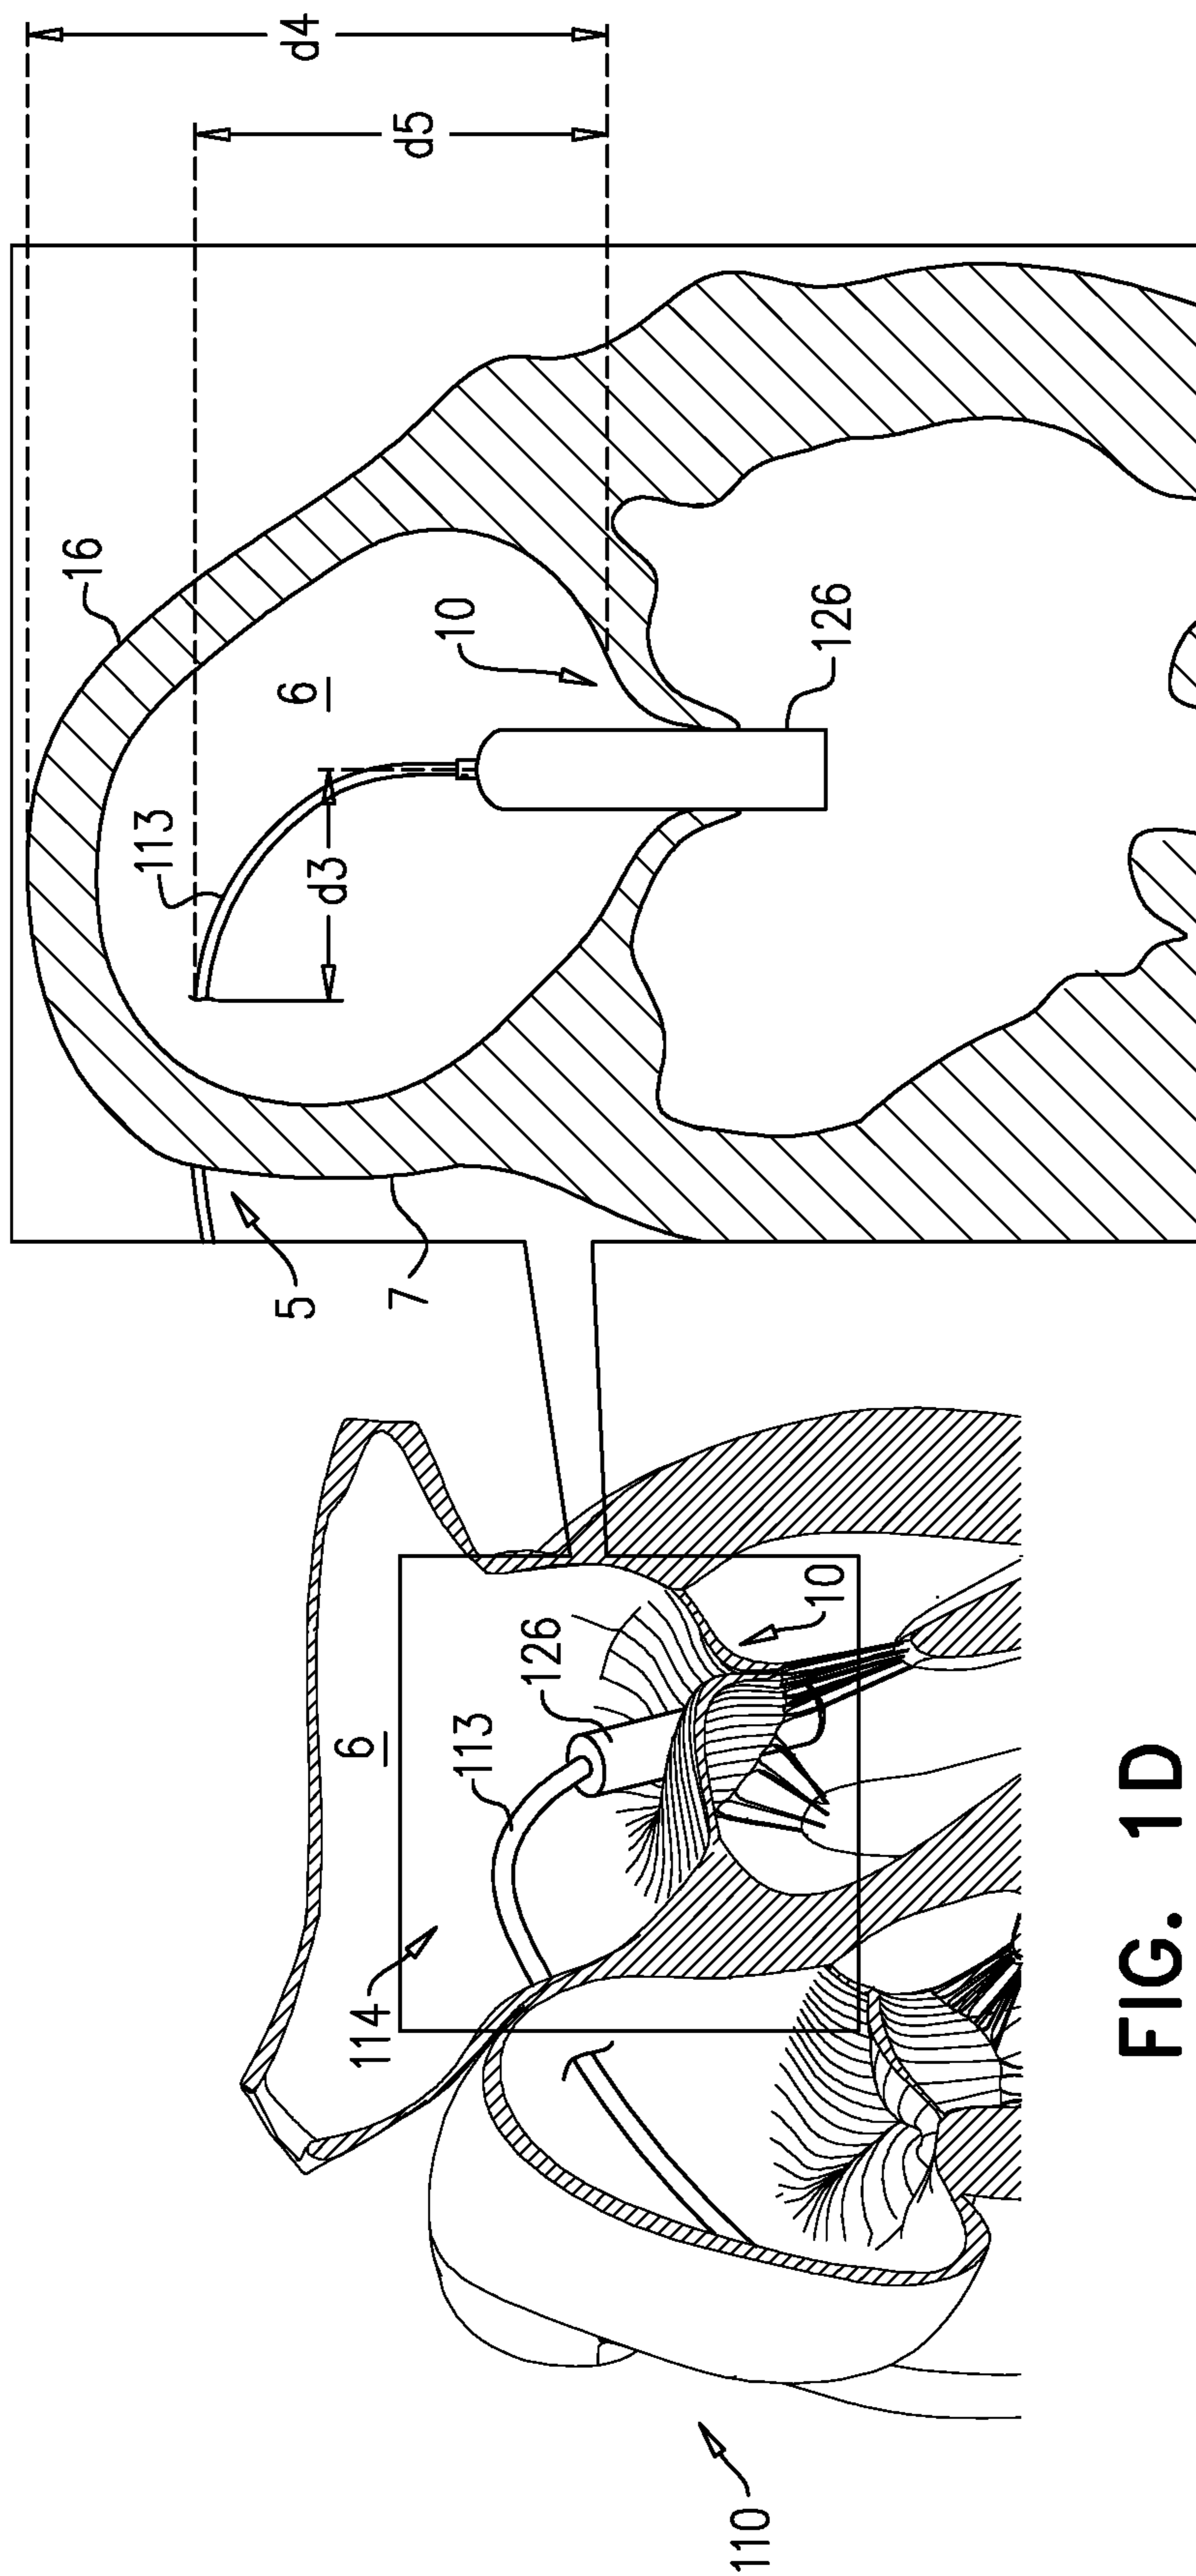


FIG. 1C







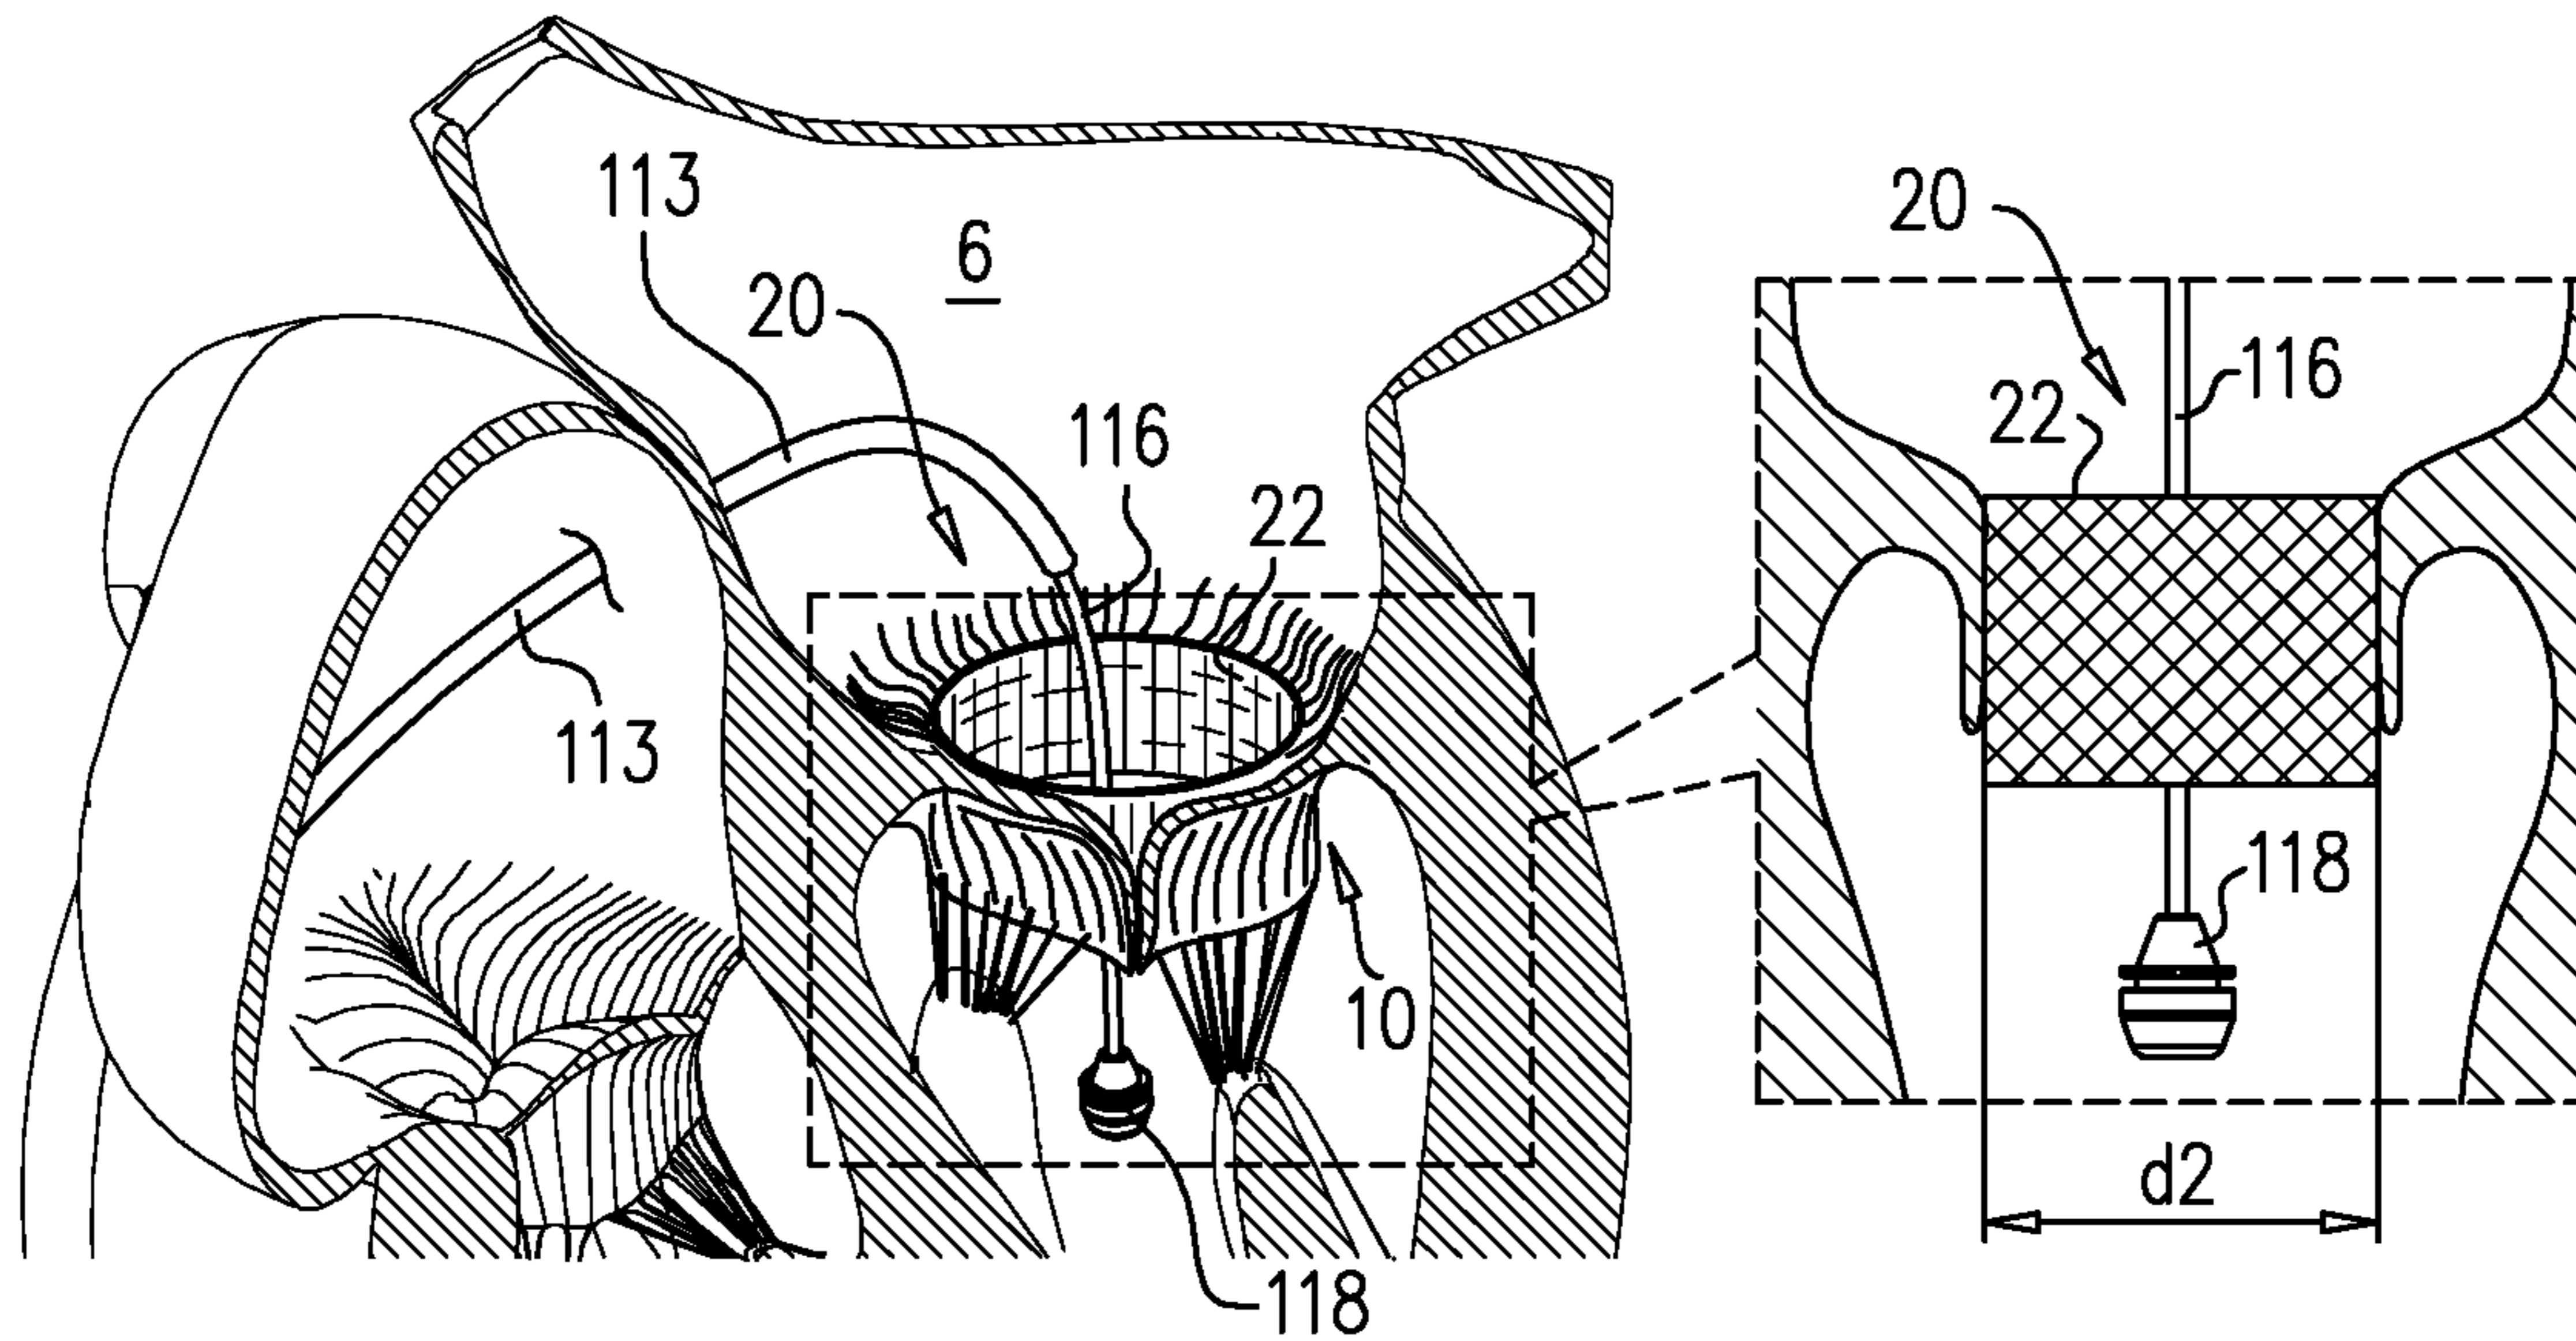


FIG. 1E

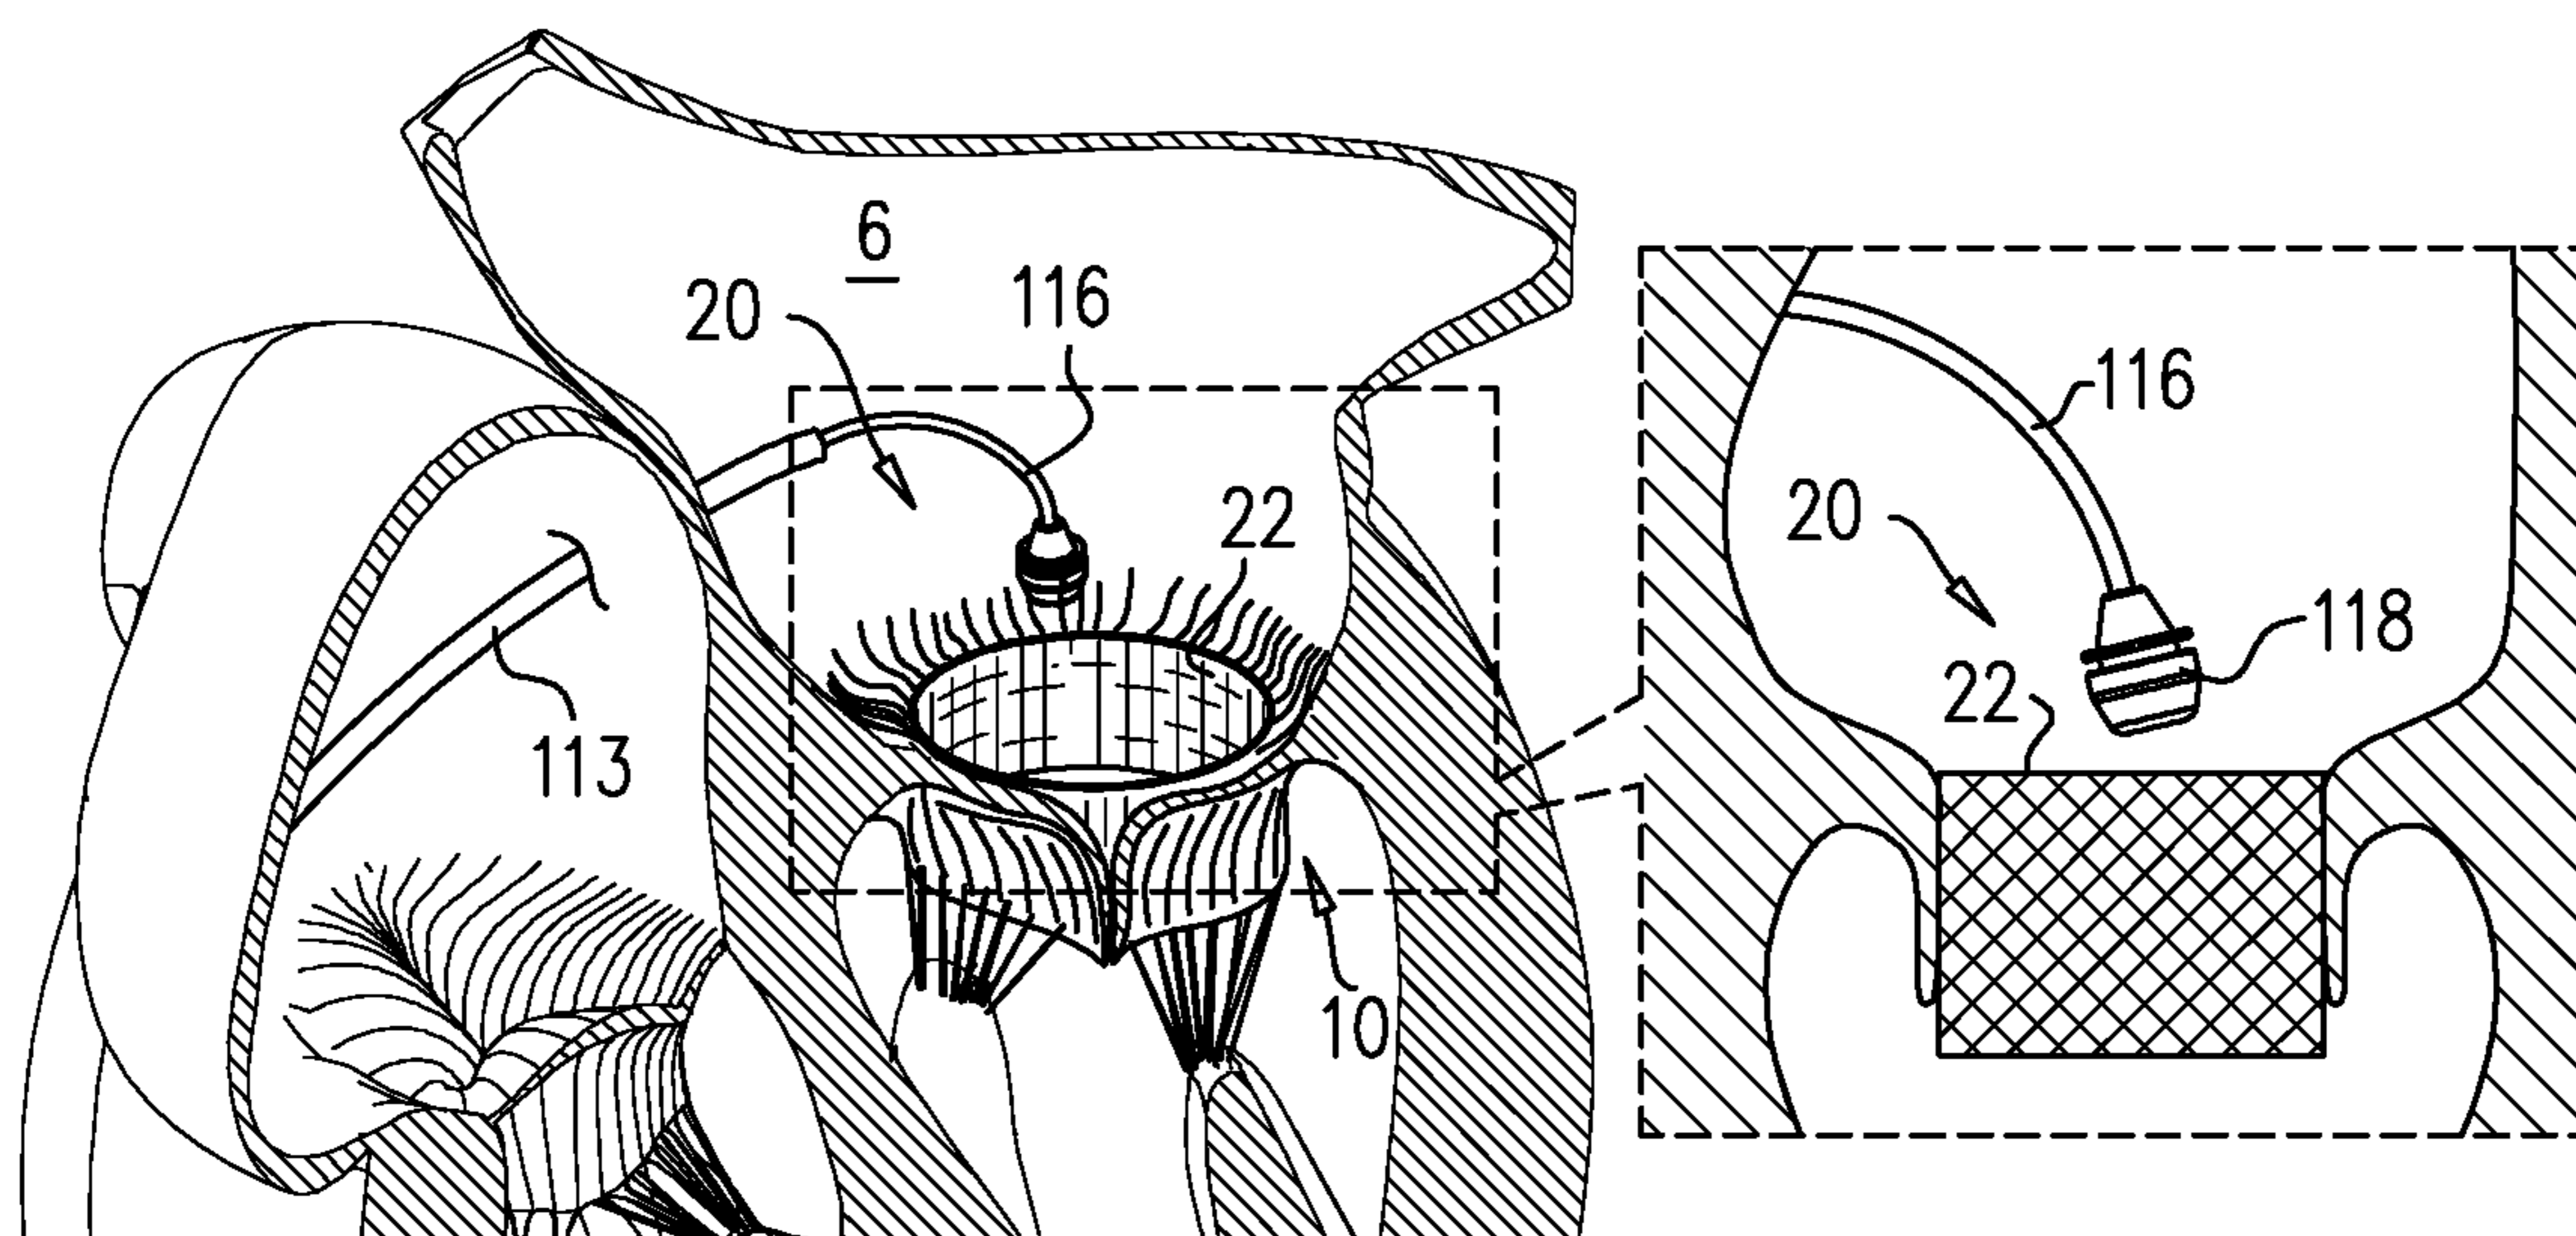


FIG. 1F

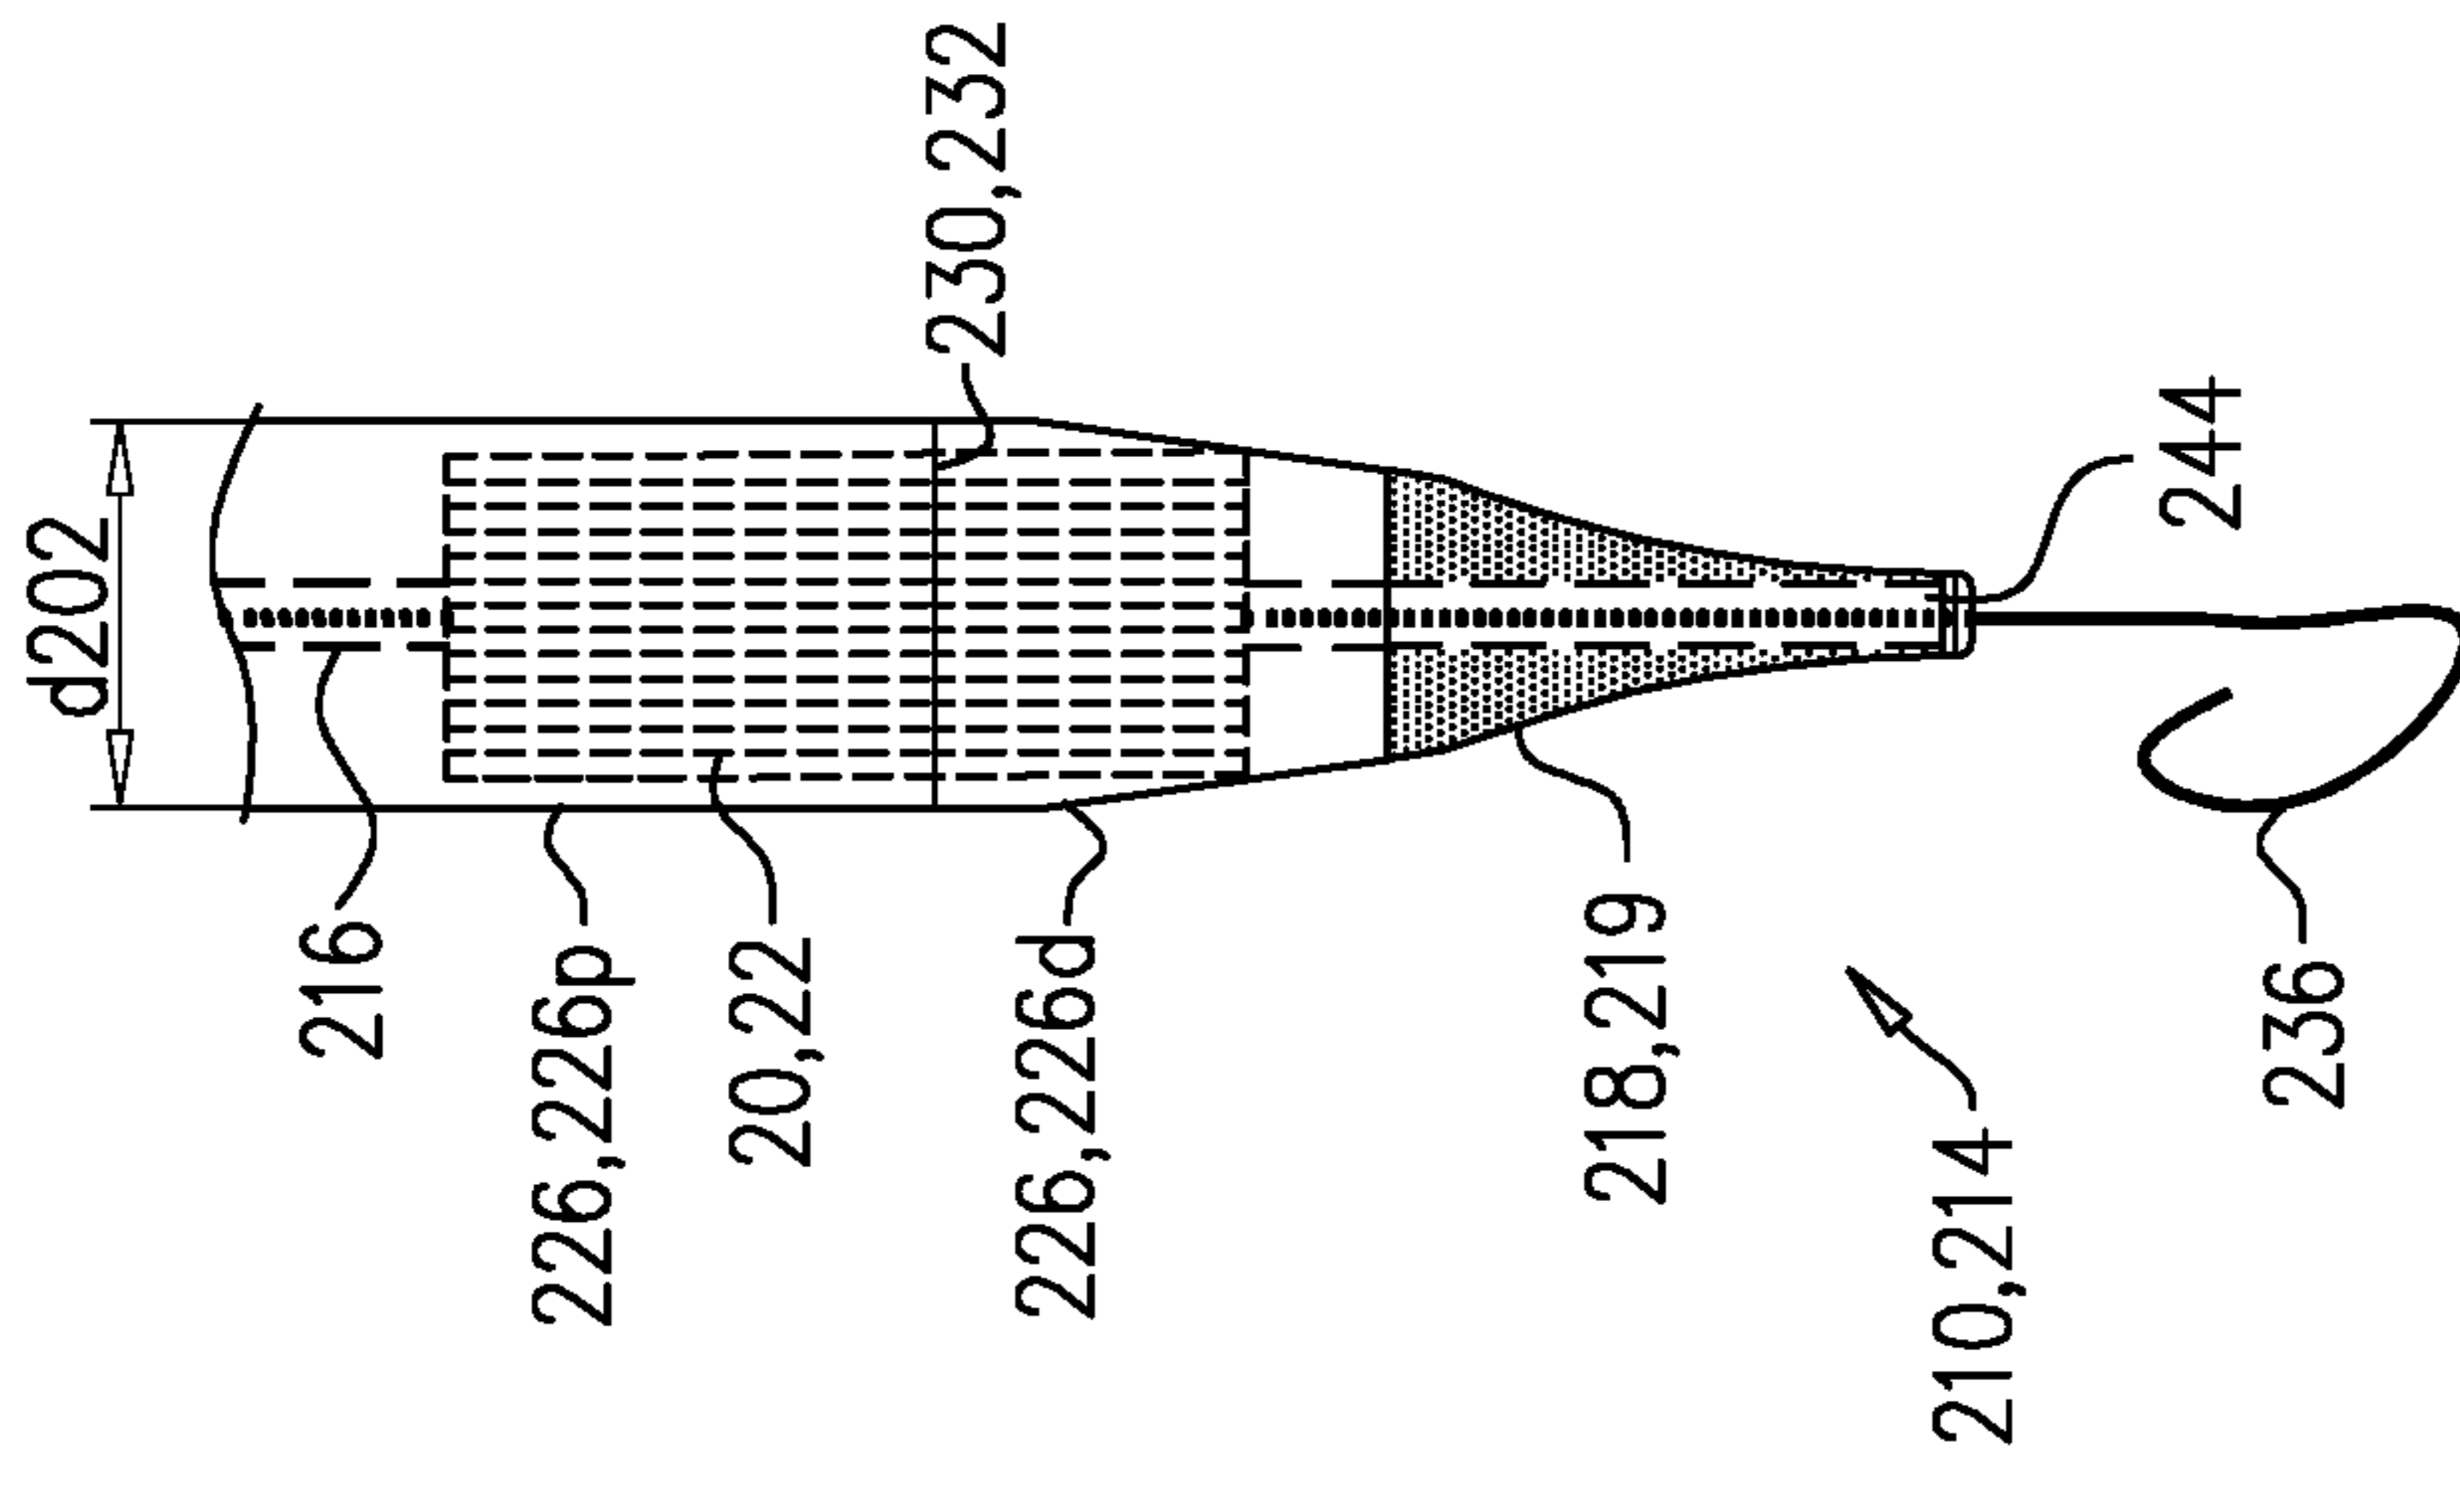


FIG. 2A

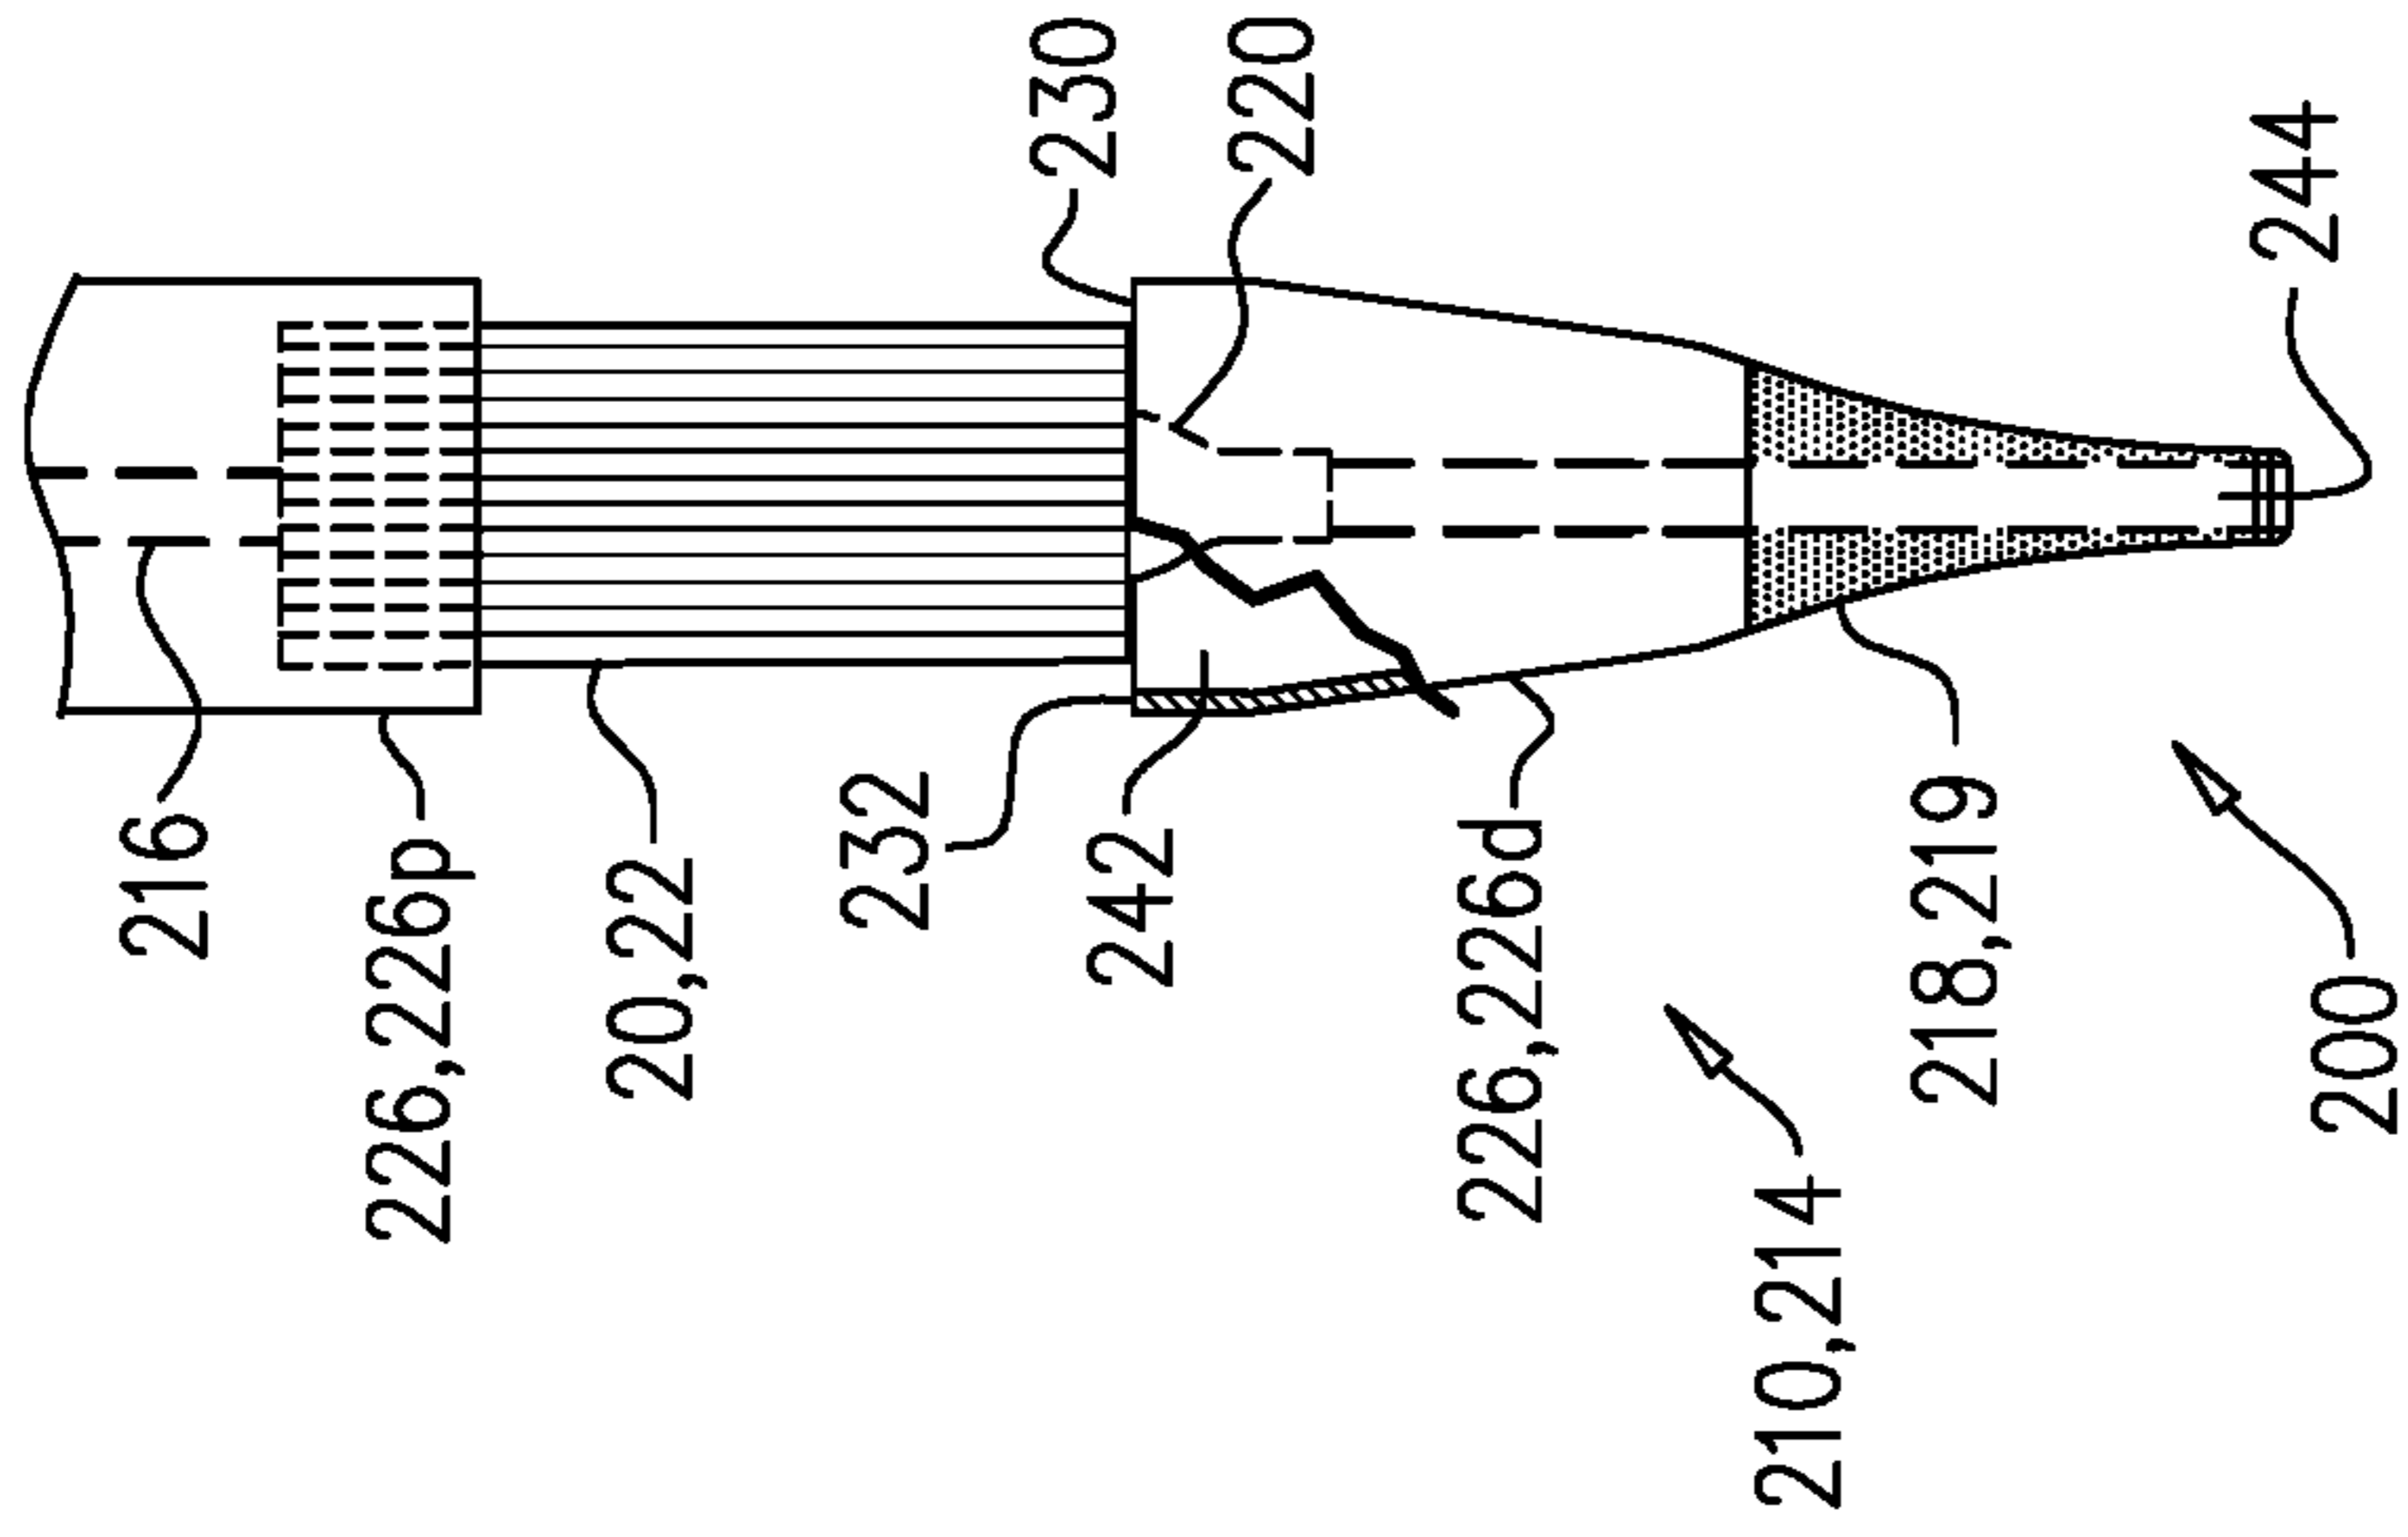


FIG. 2B

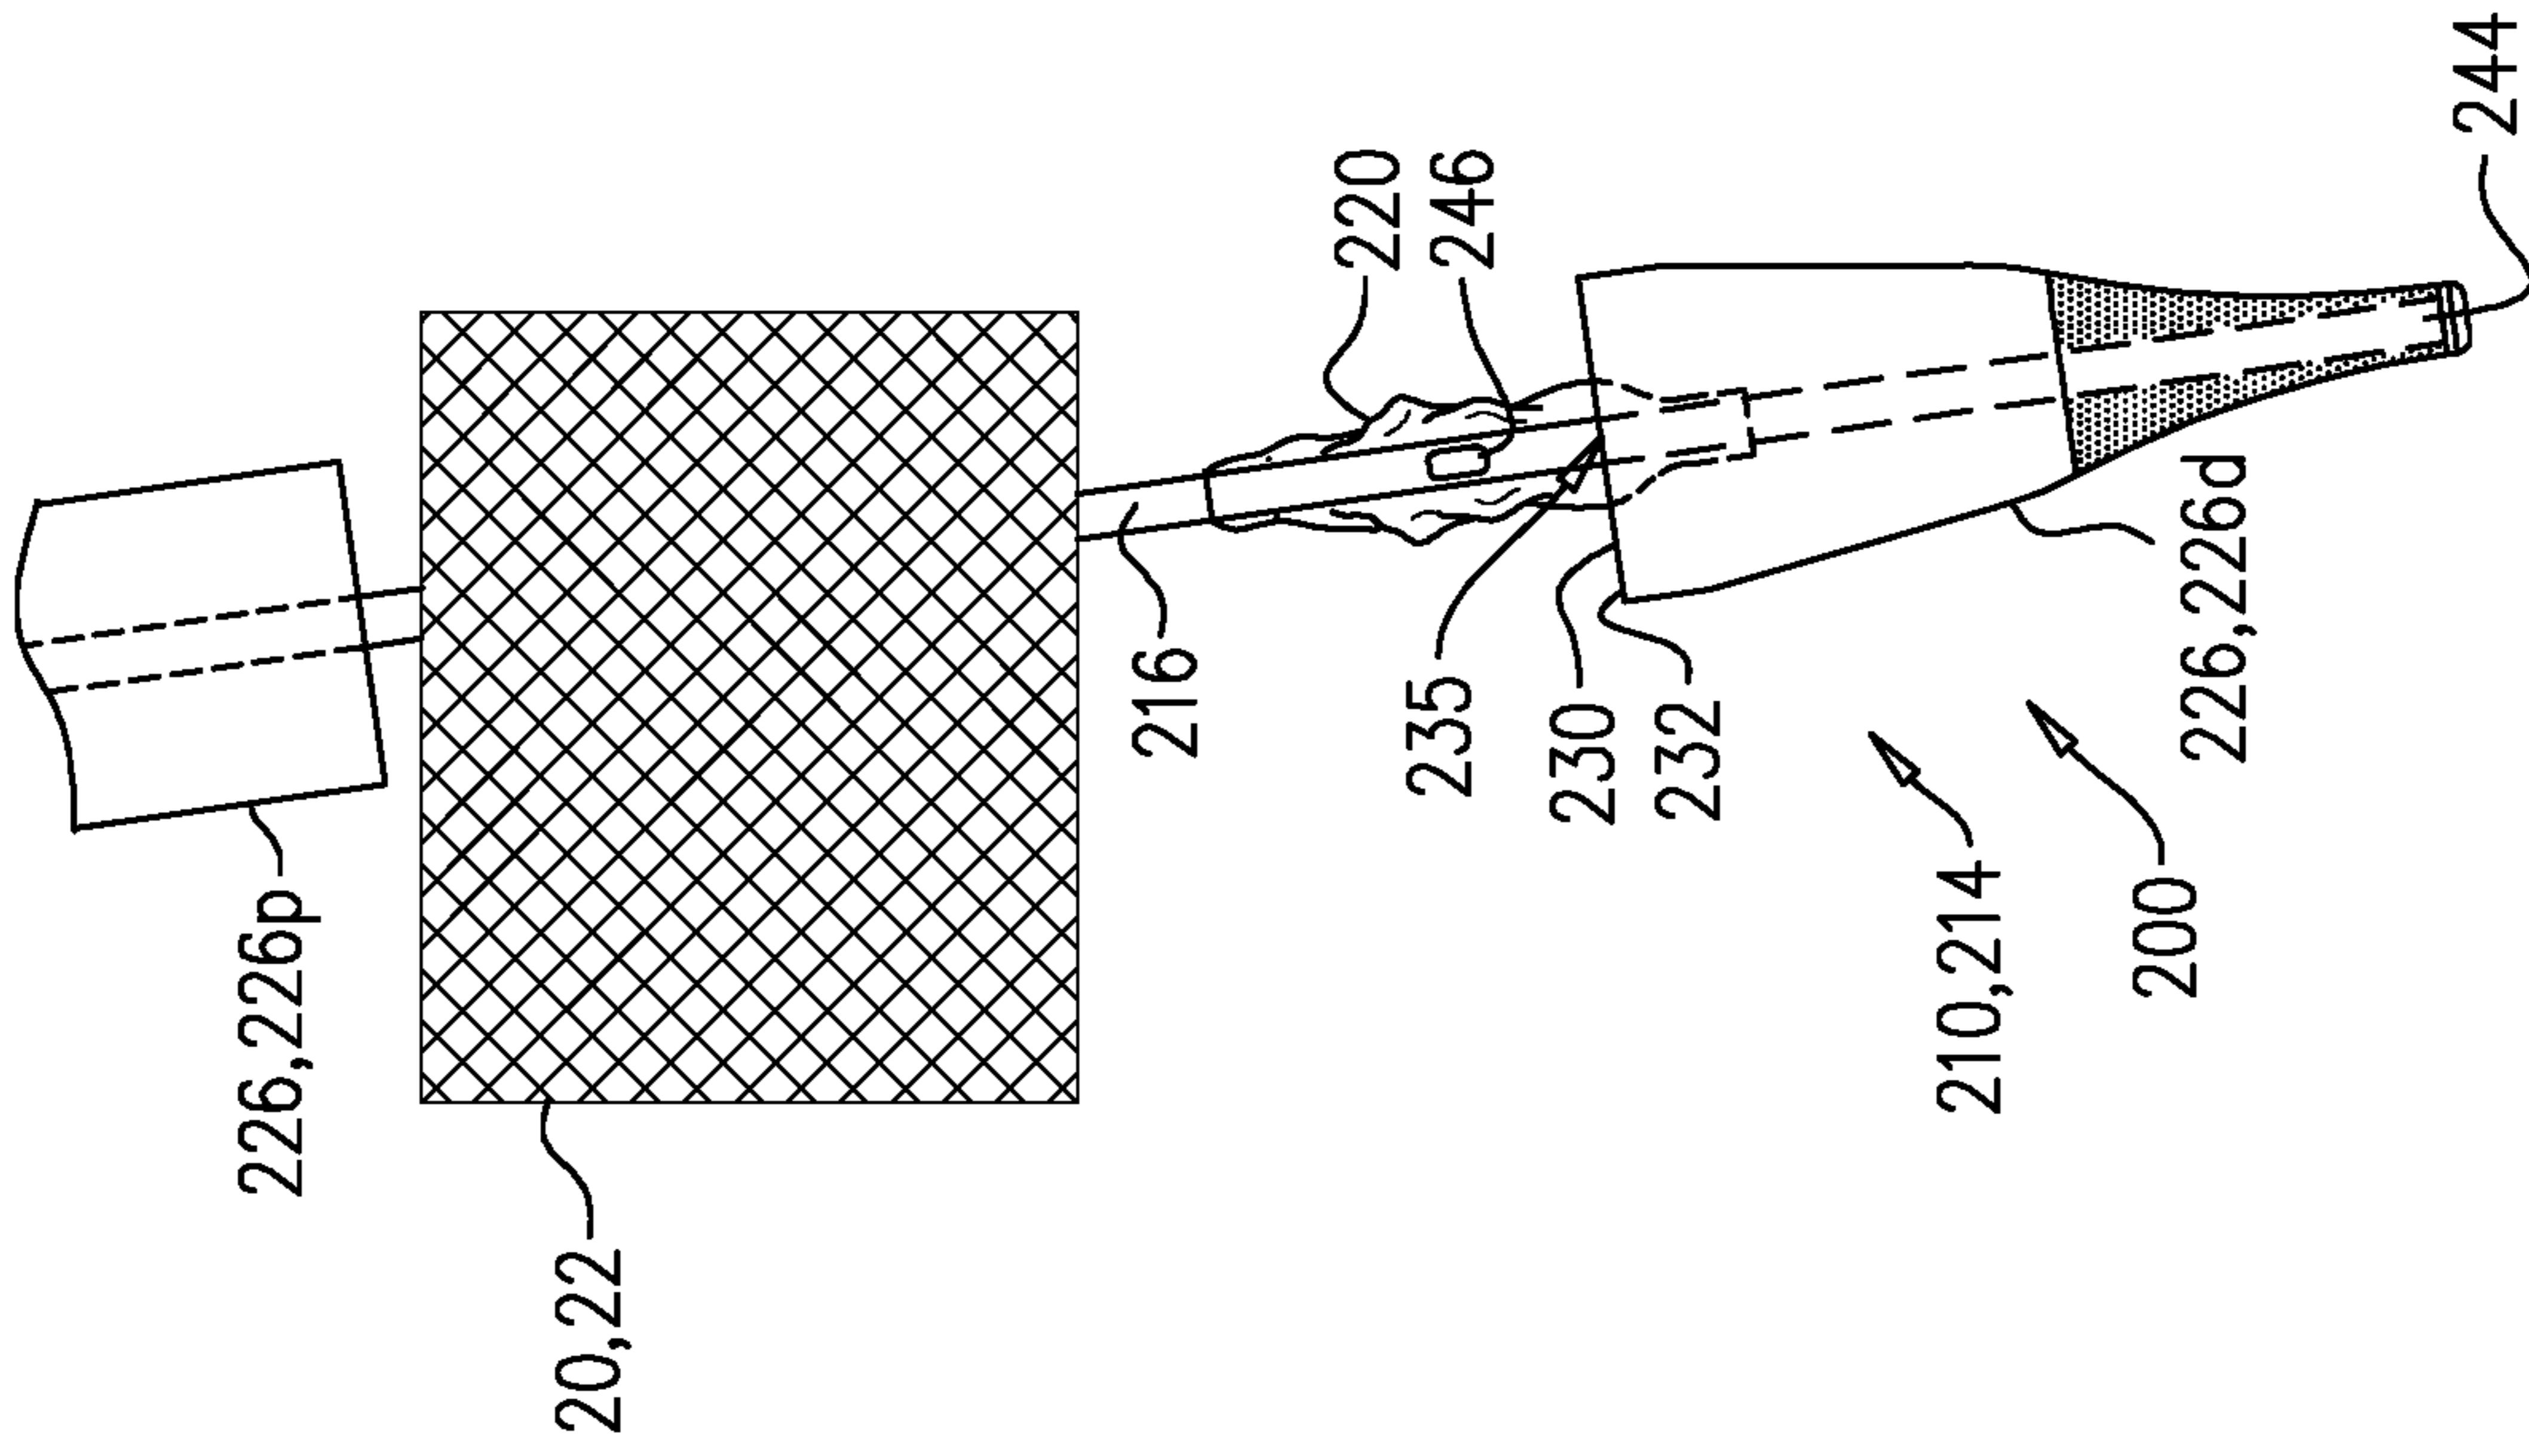


FIG. 2C



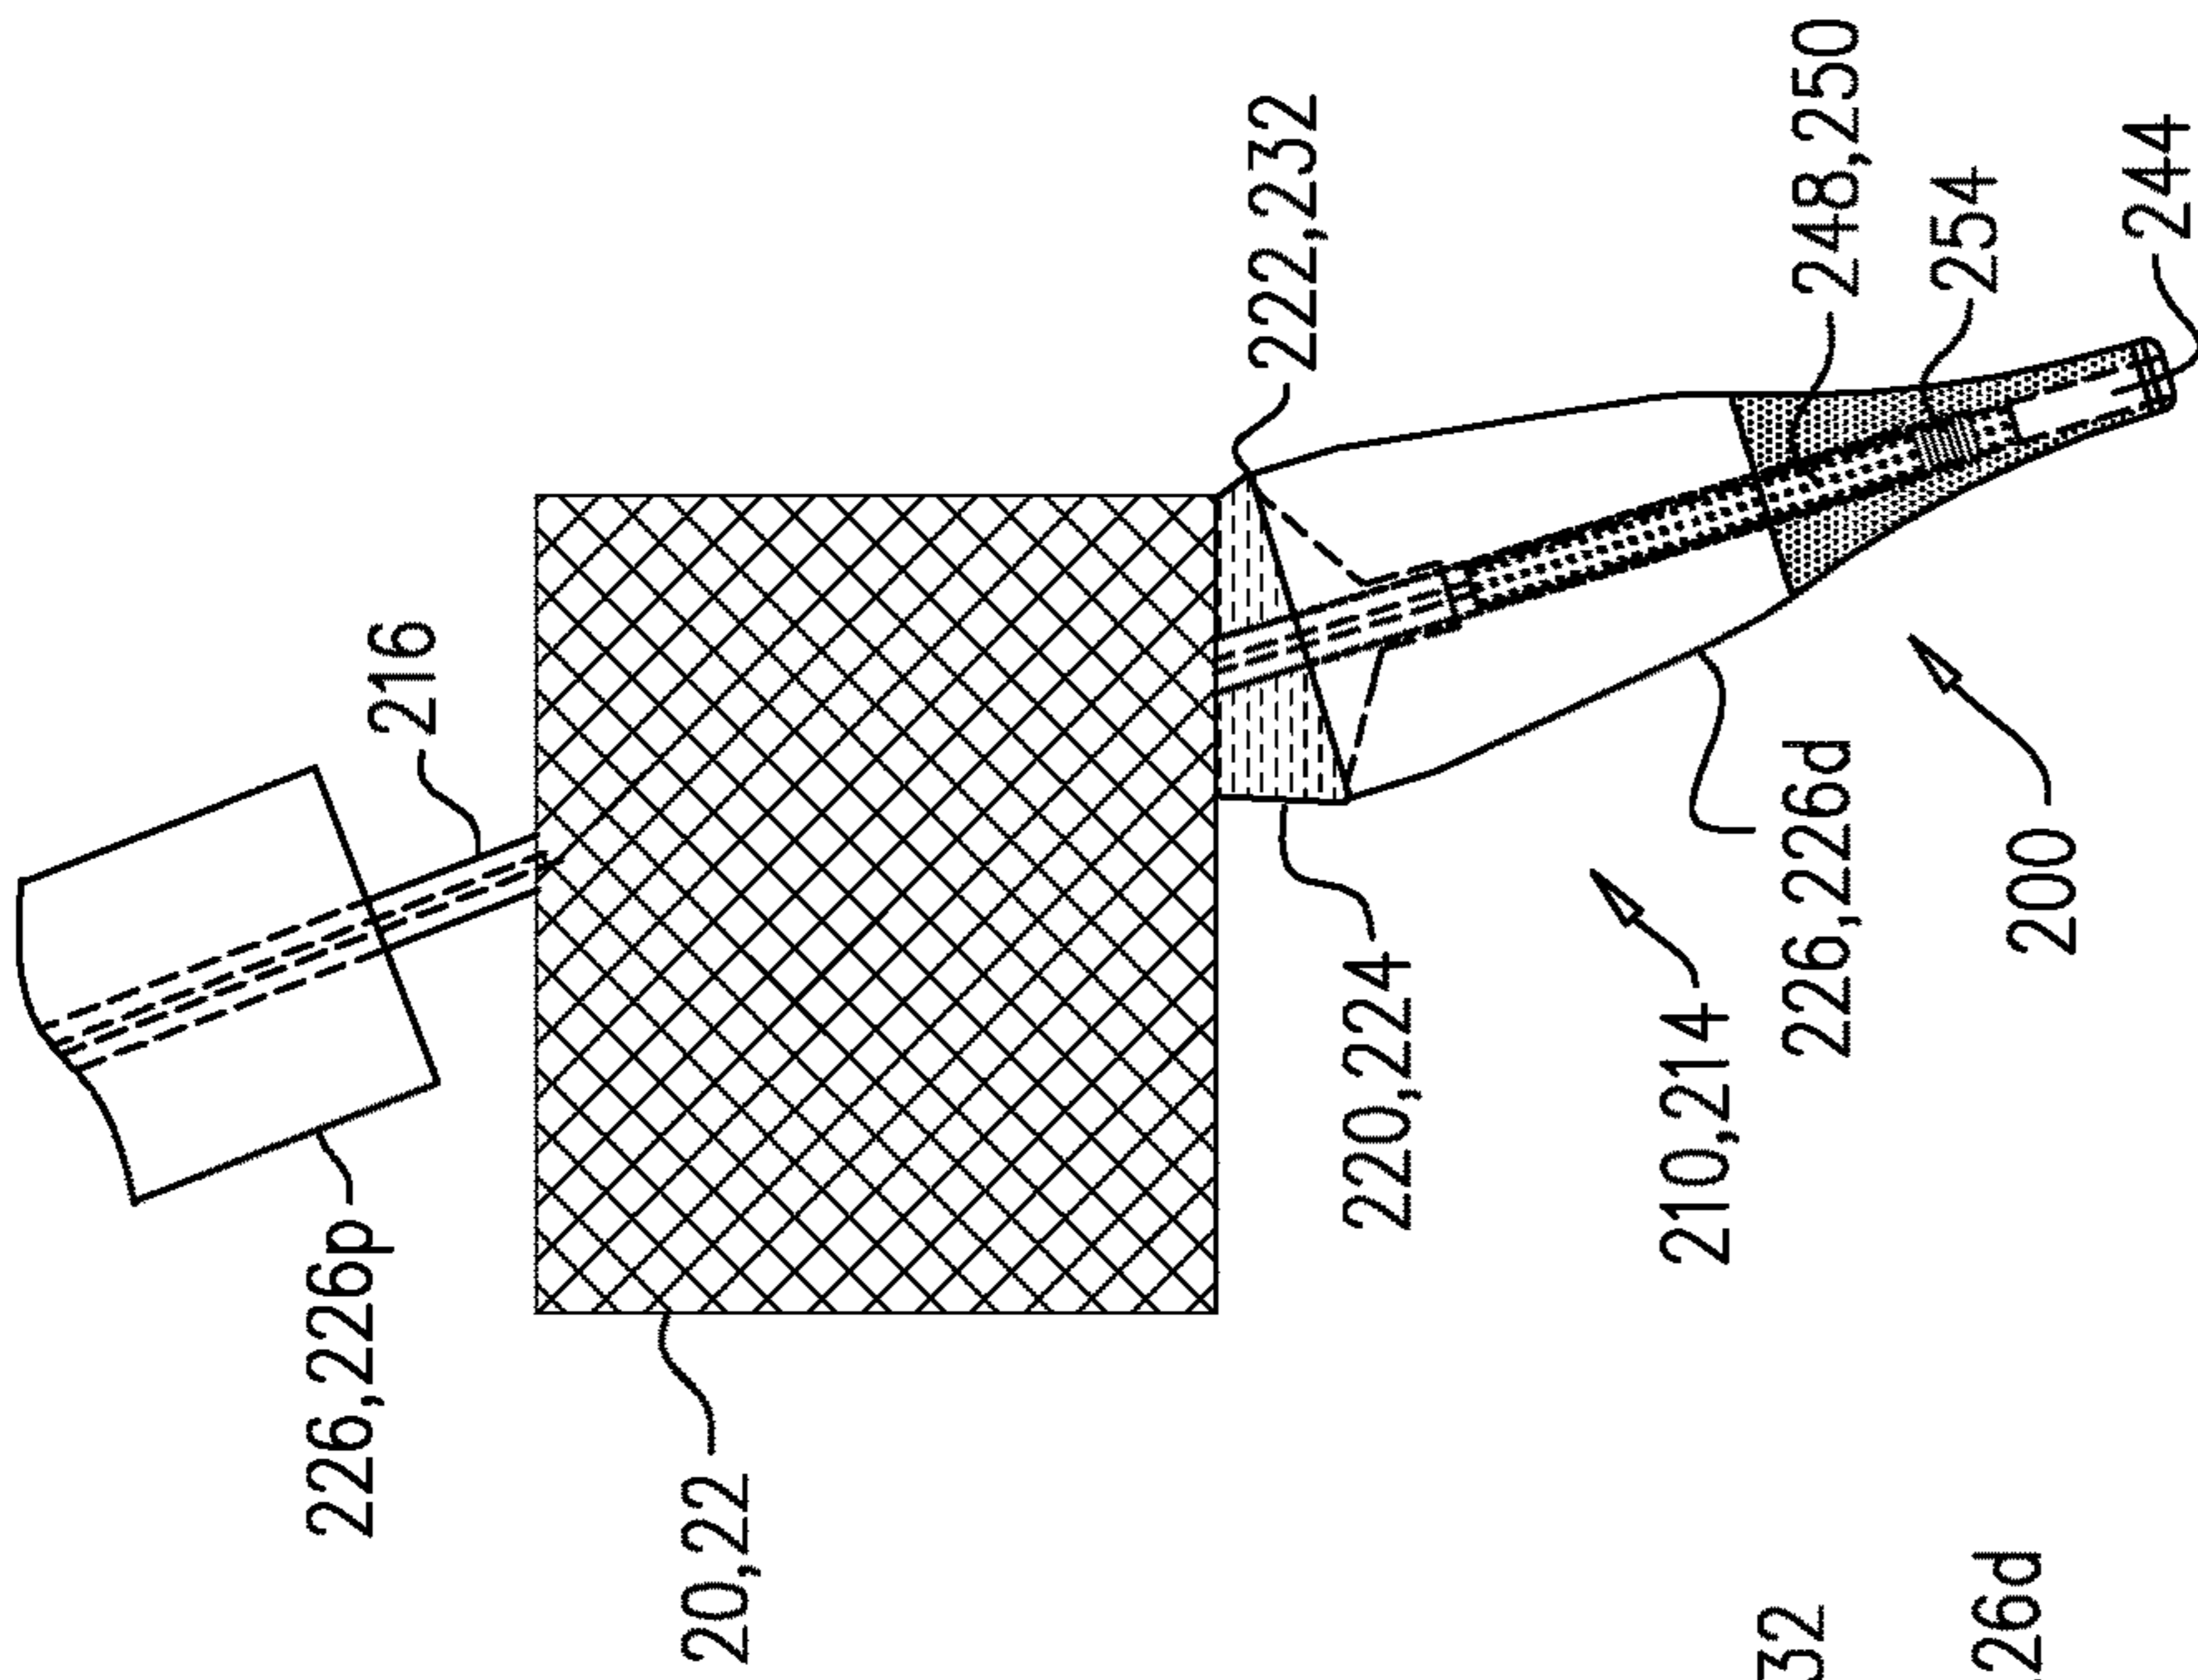


FIG. 2D

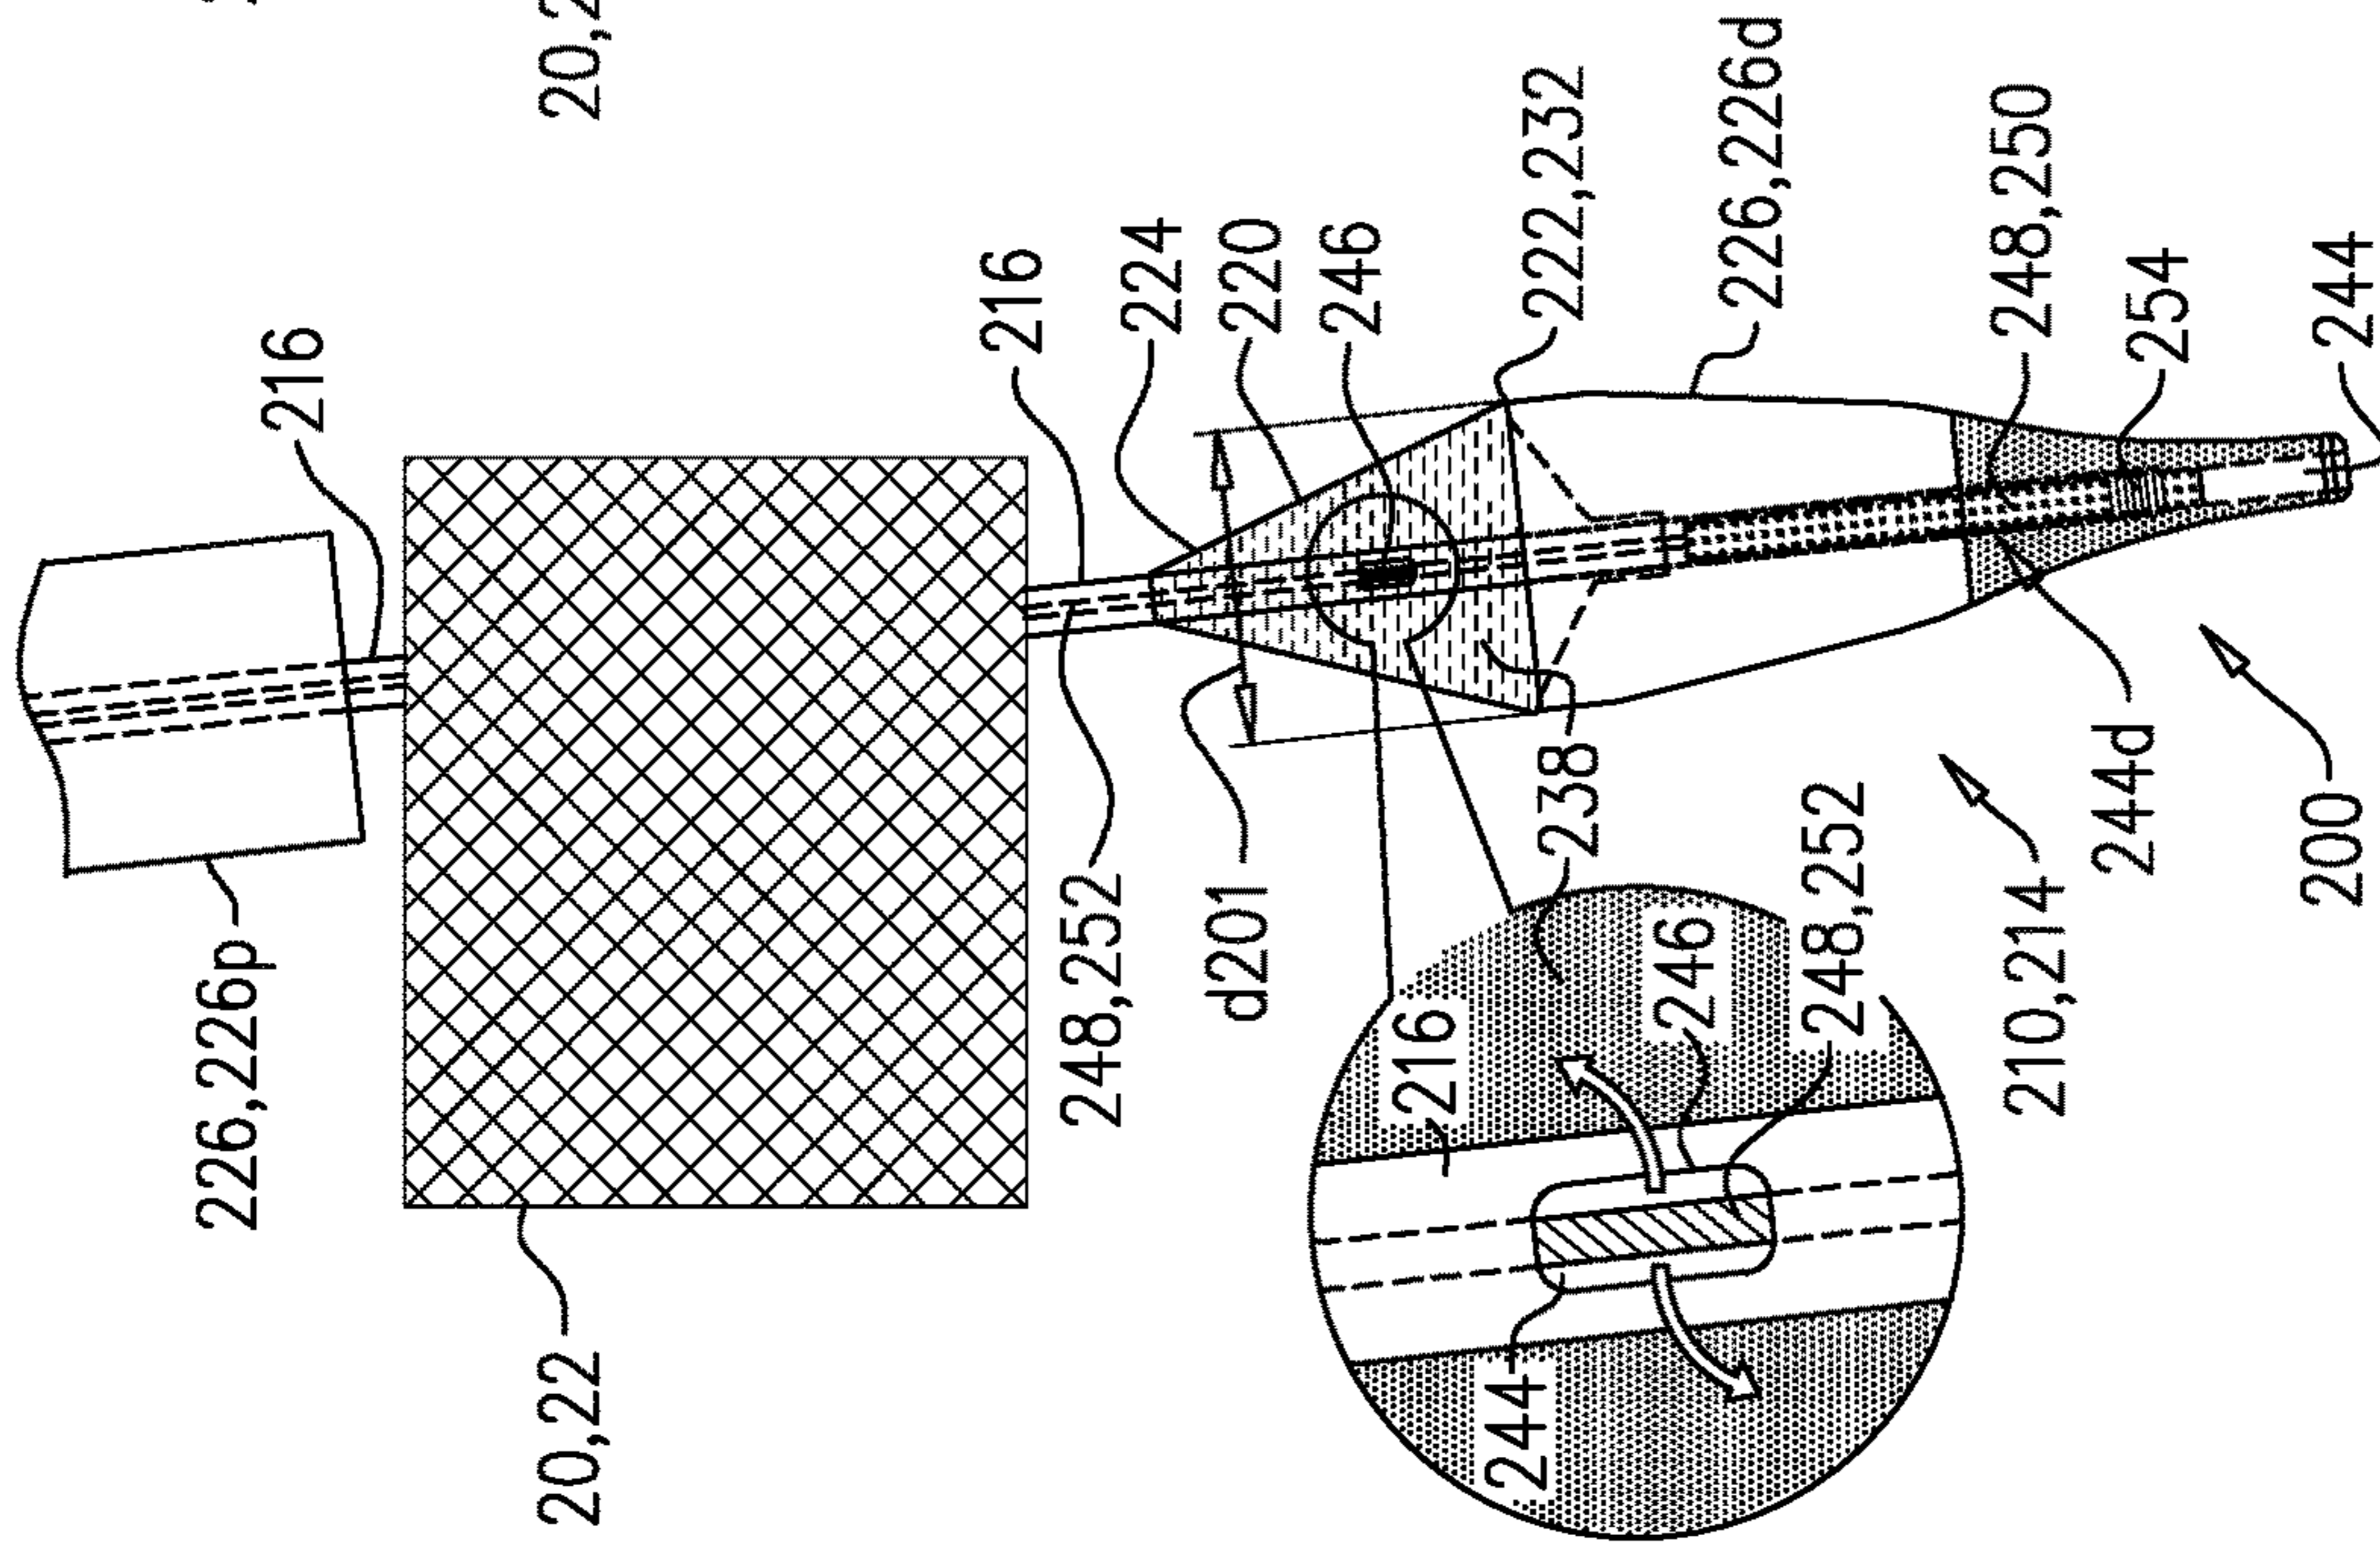


FIG. 2E

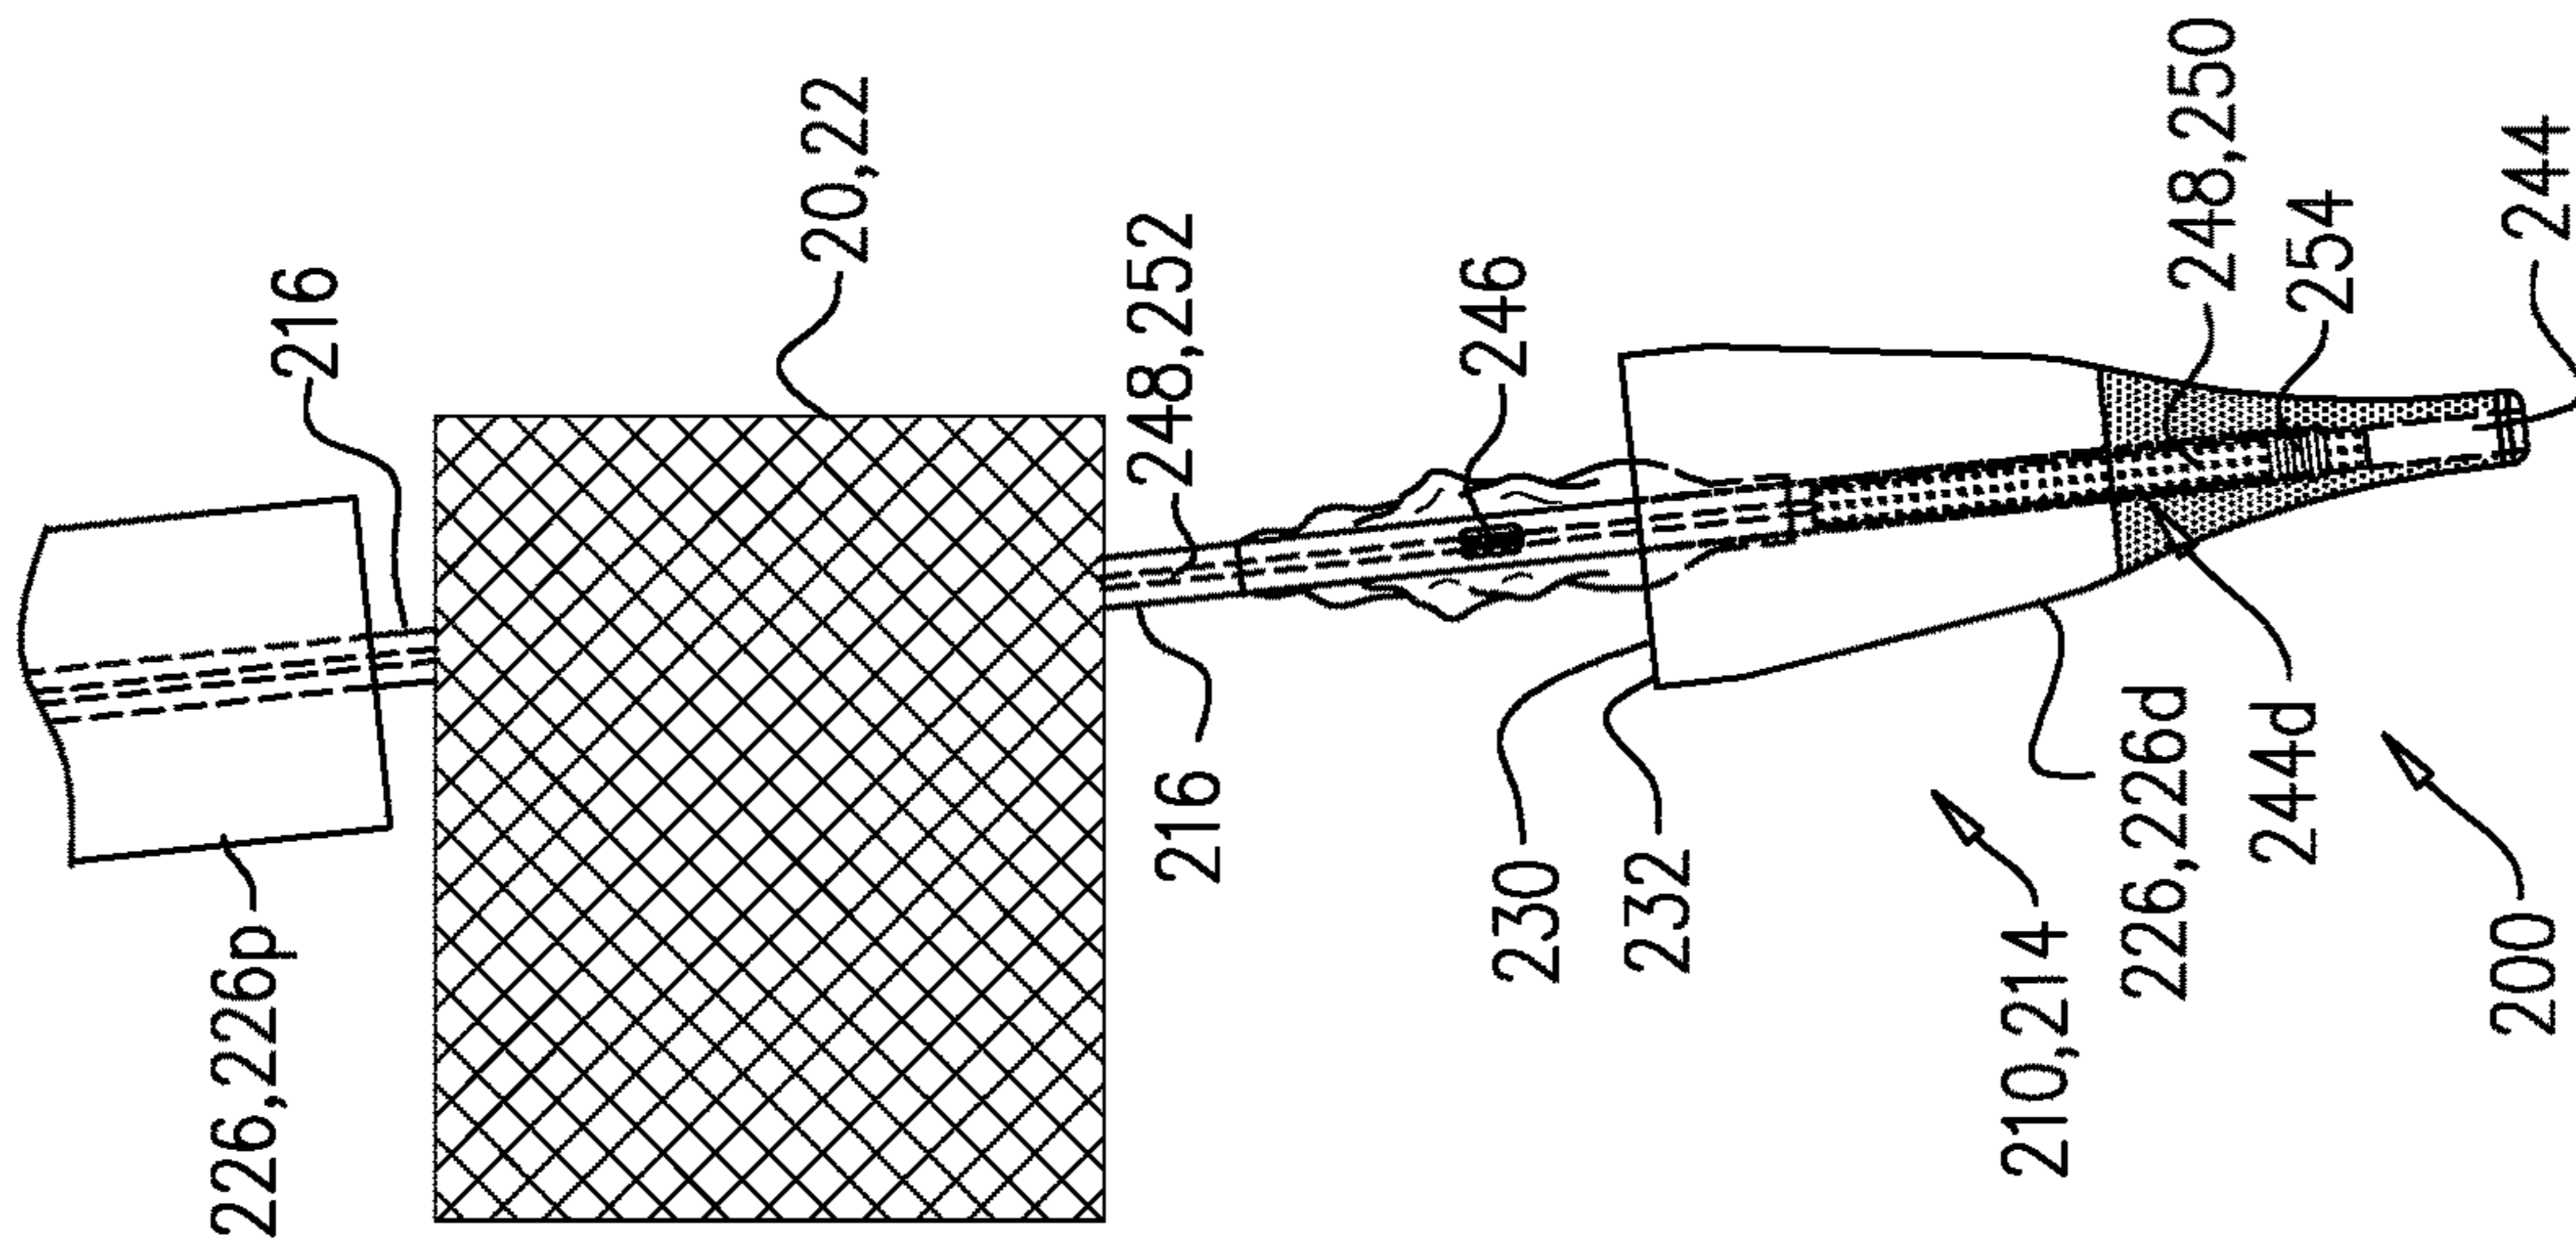


FIG. 2F

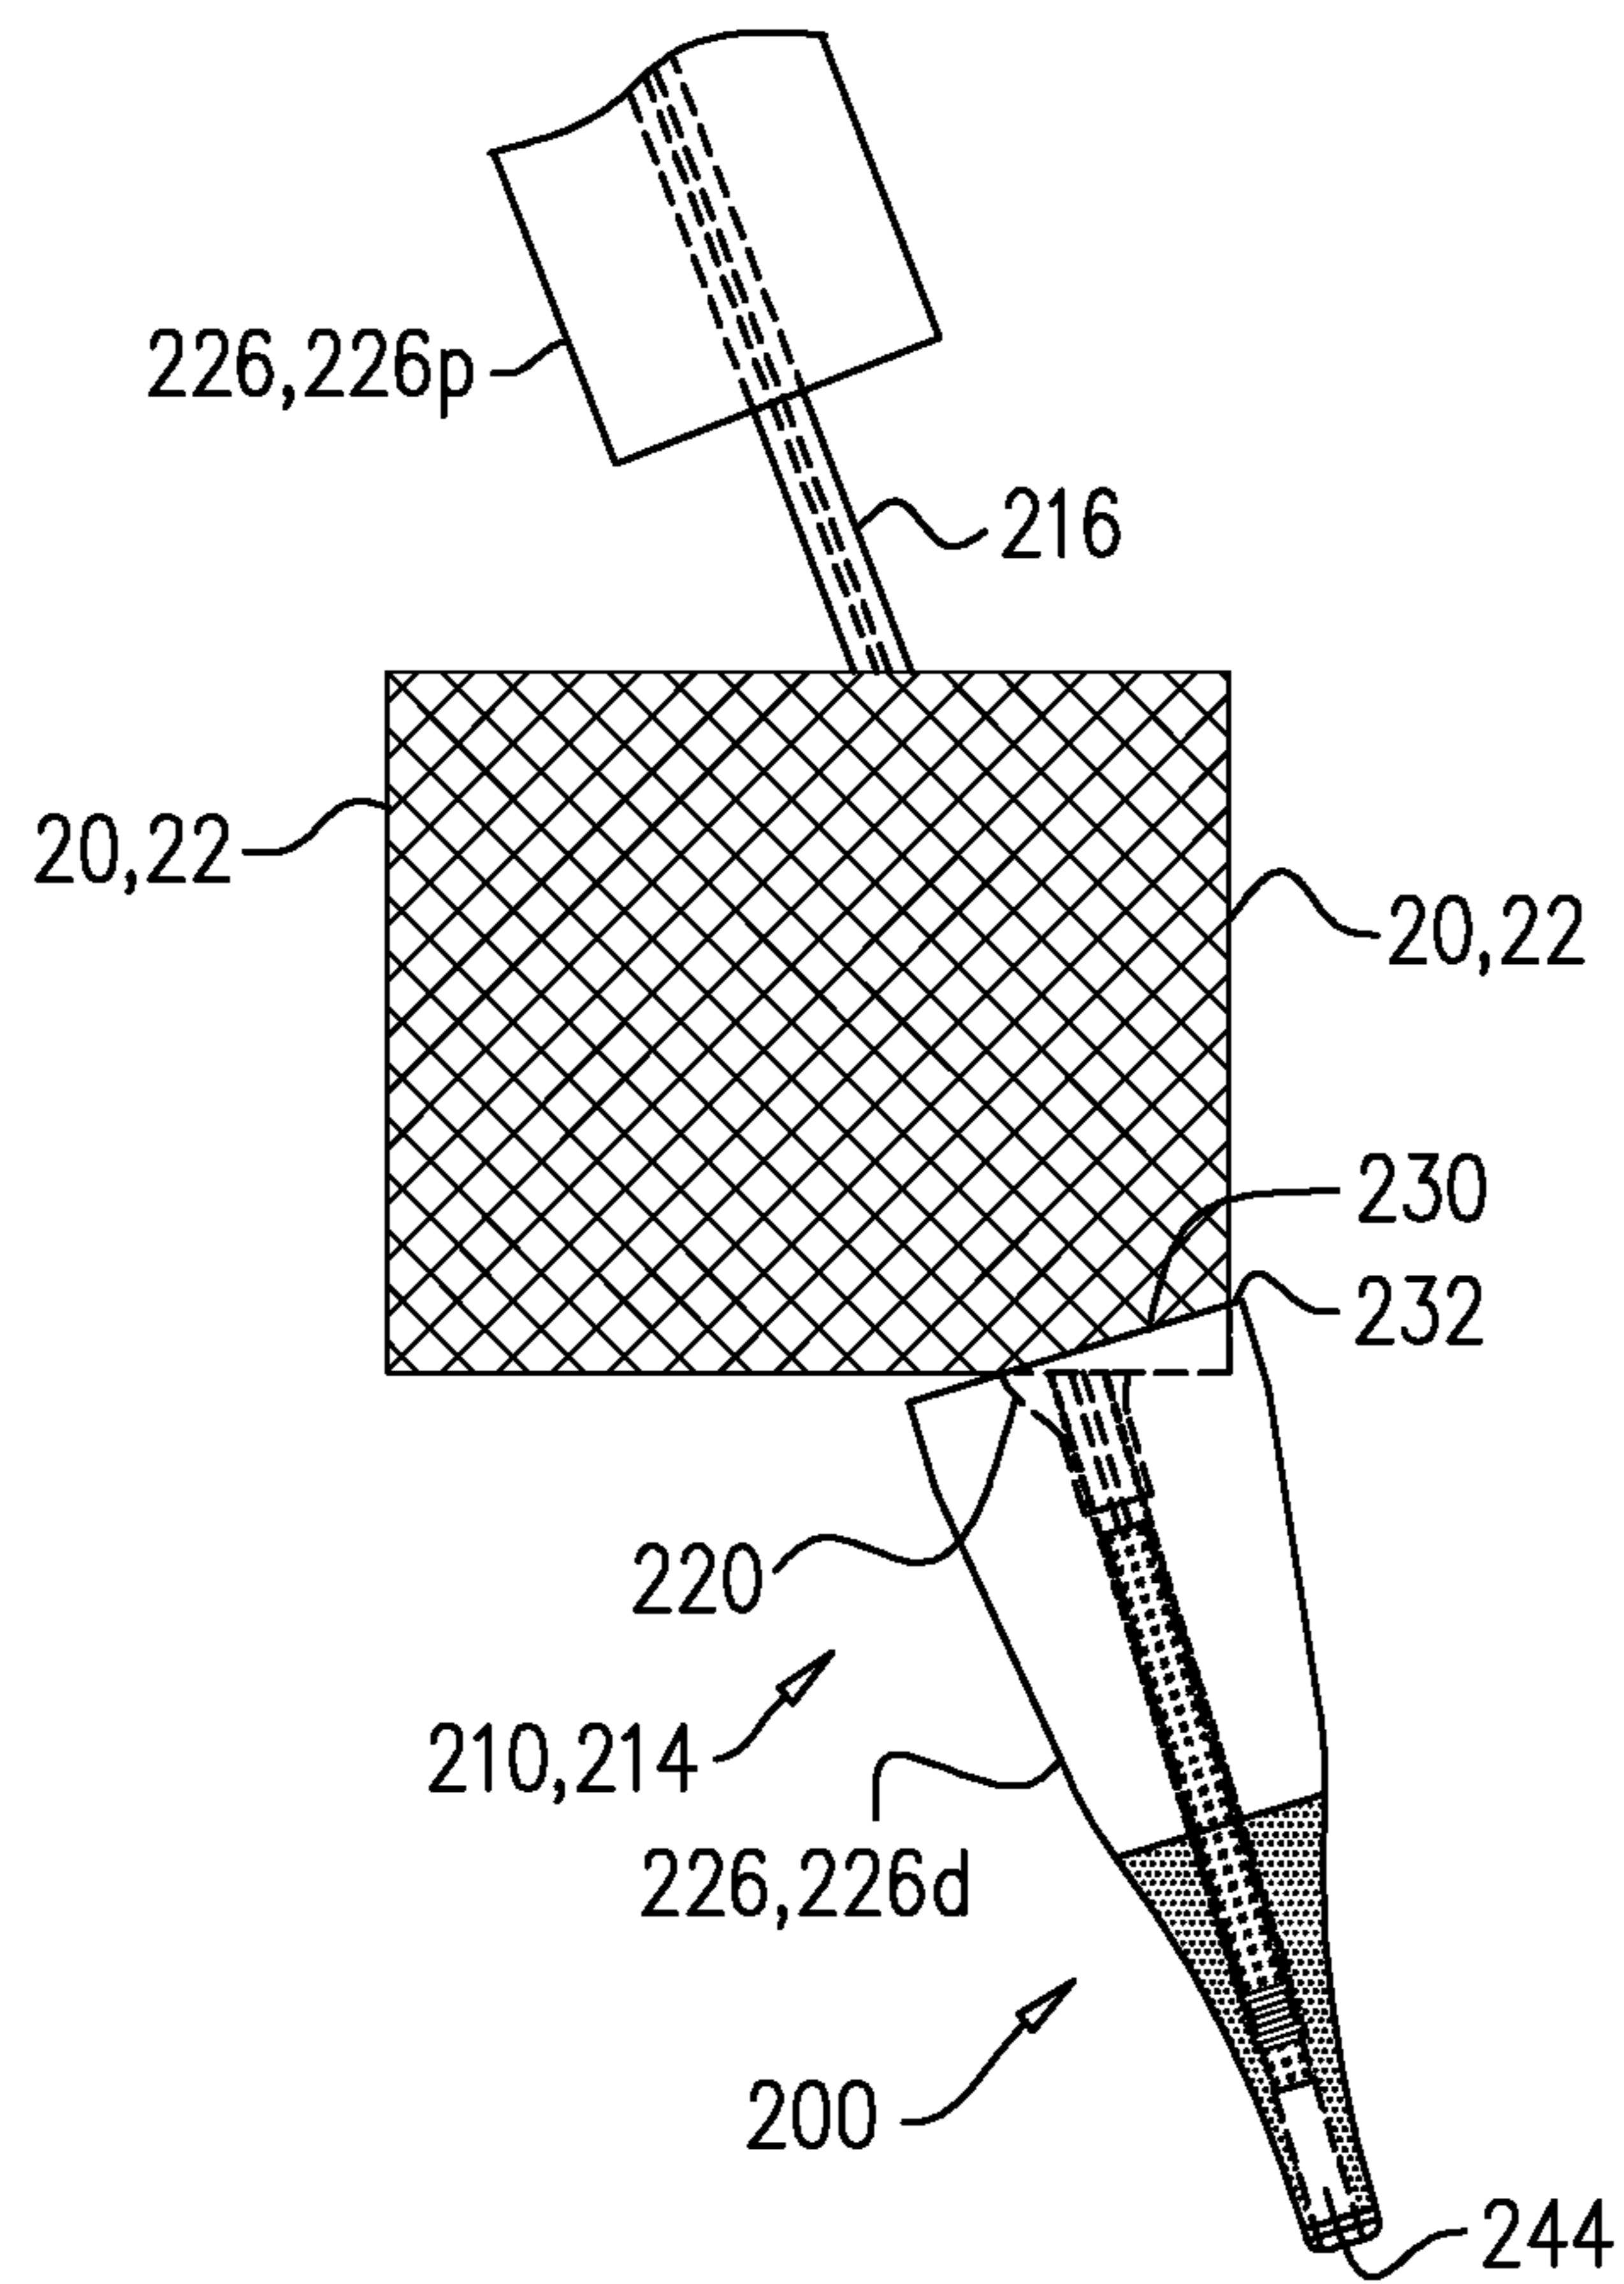


FIG. 3



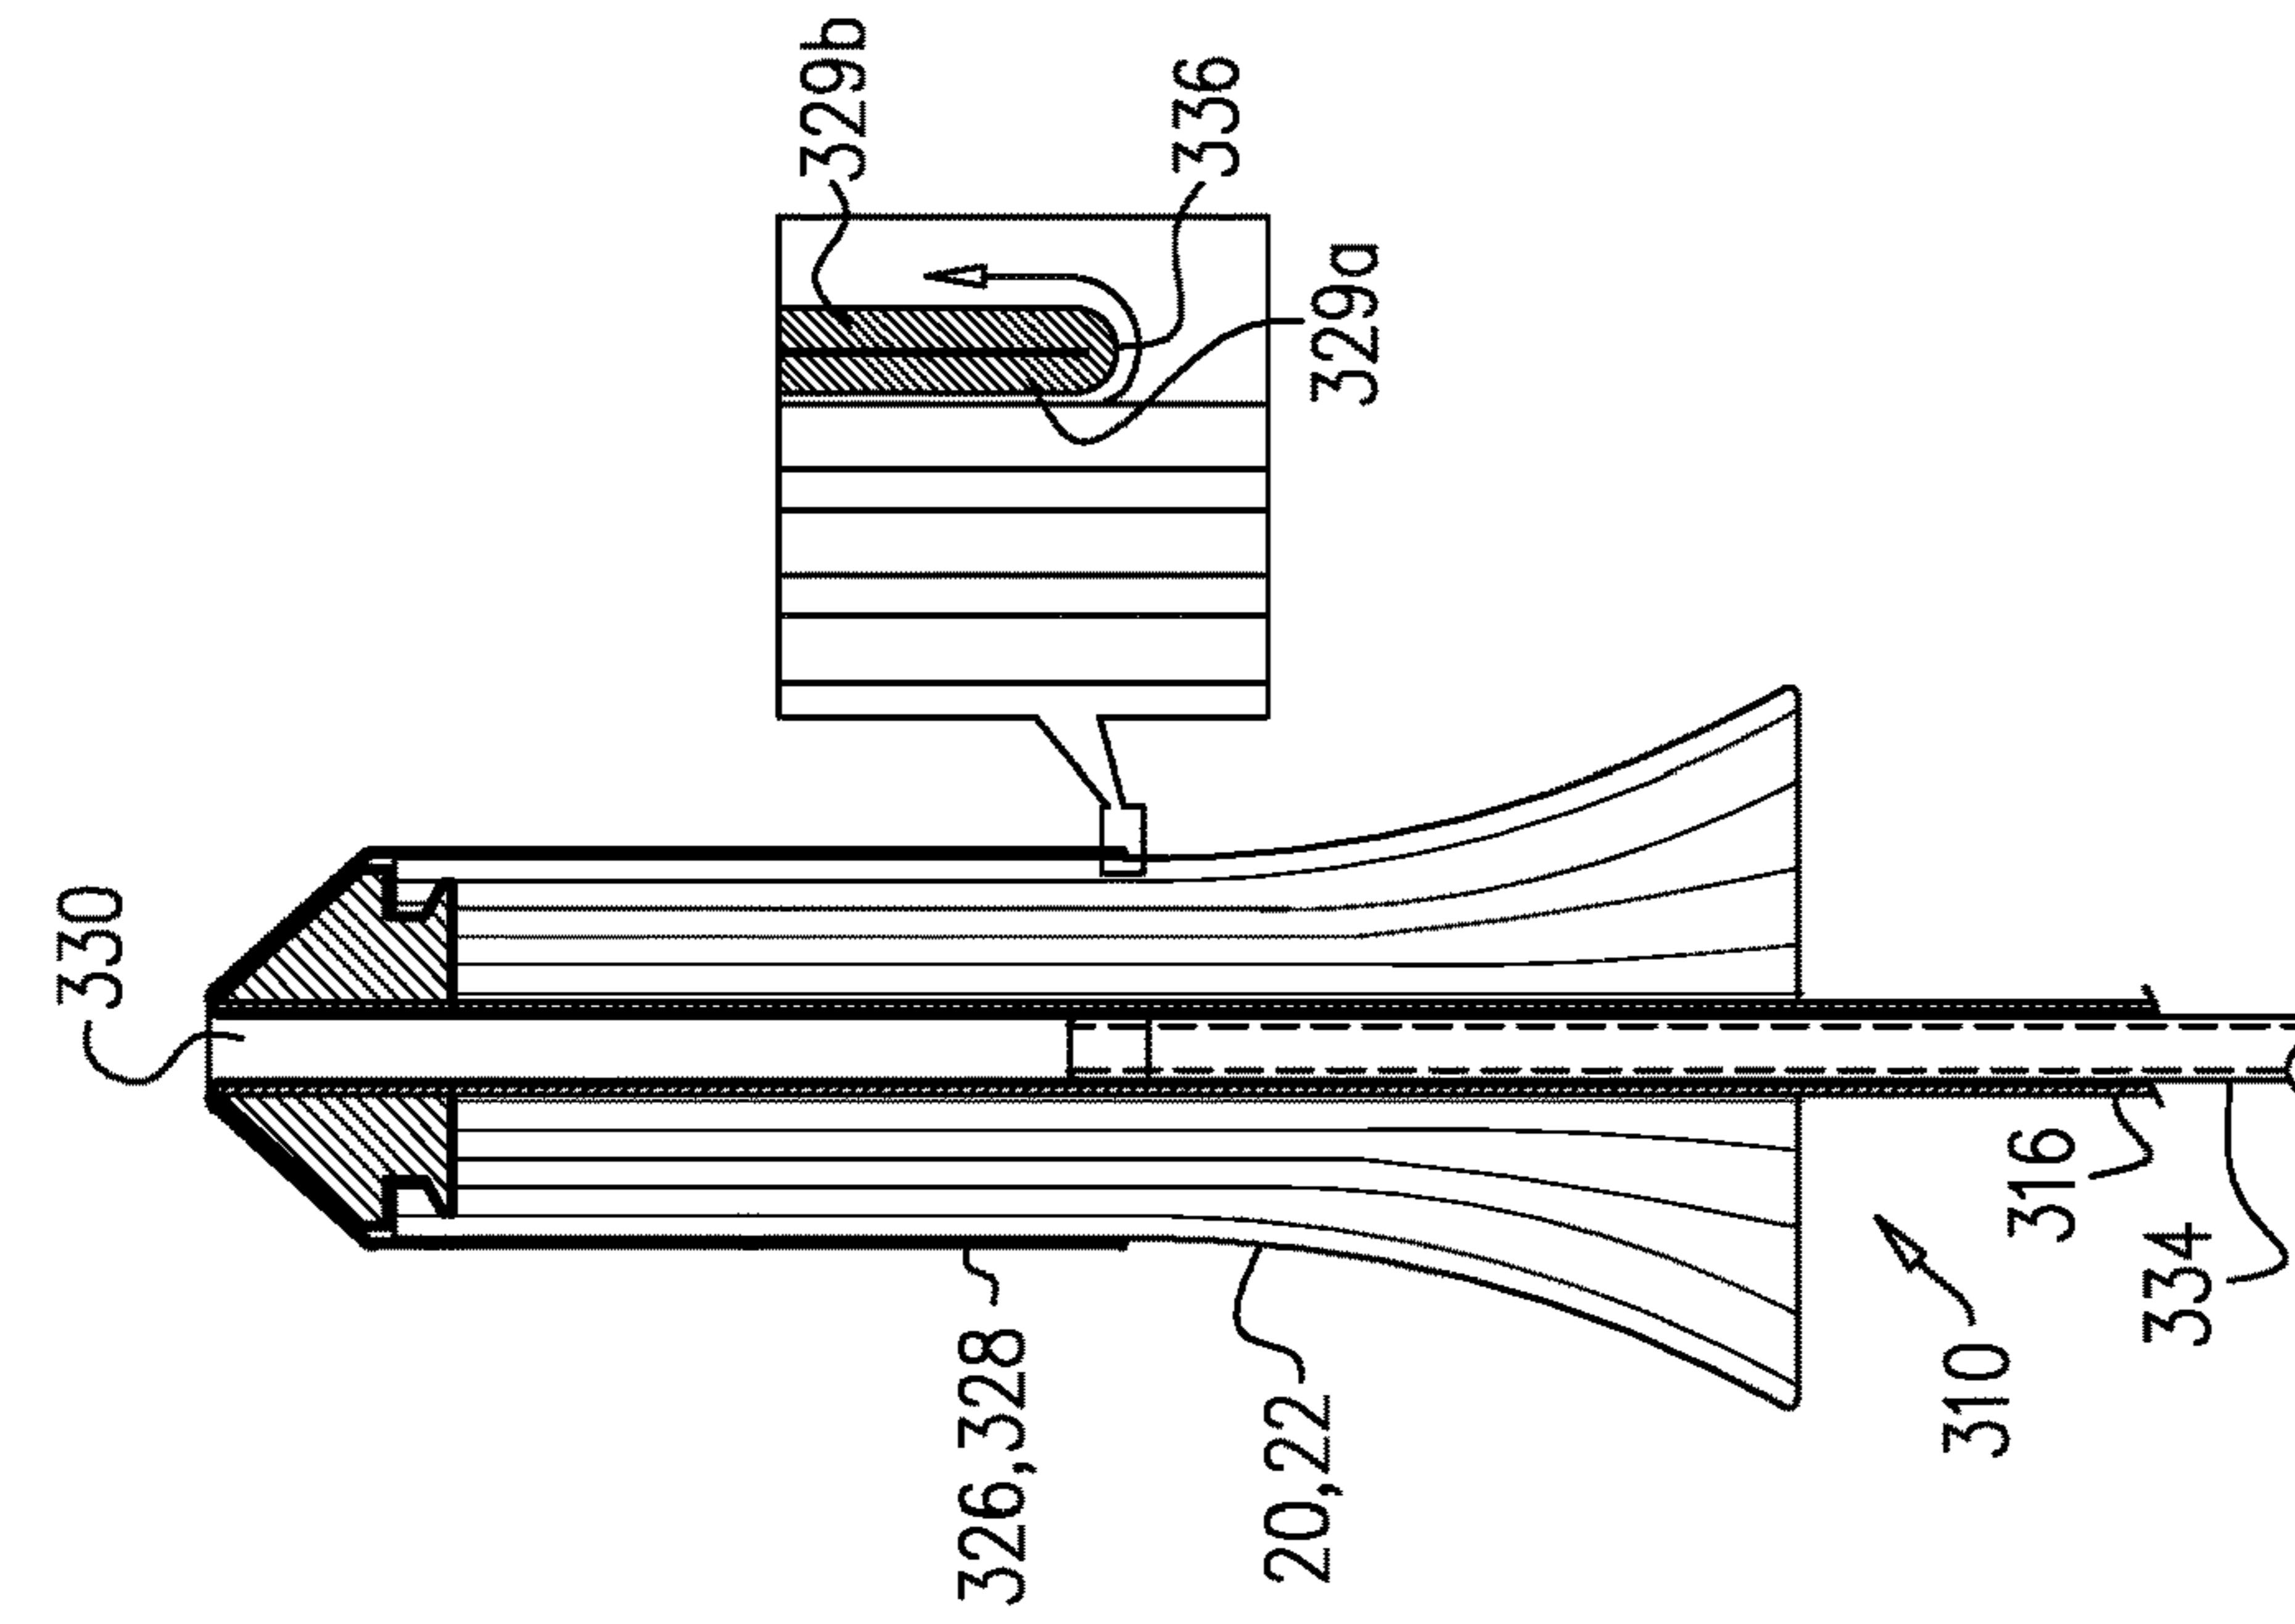


FIG. 4B

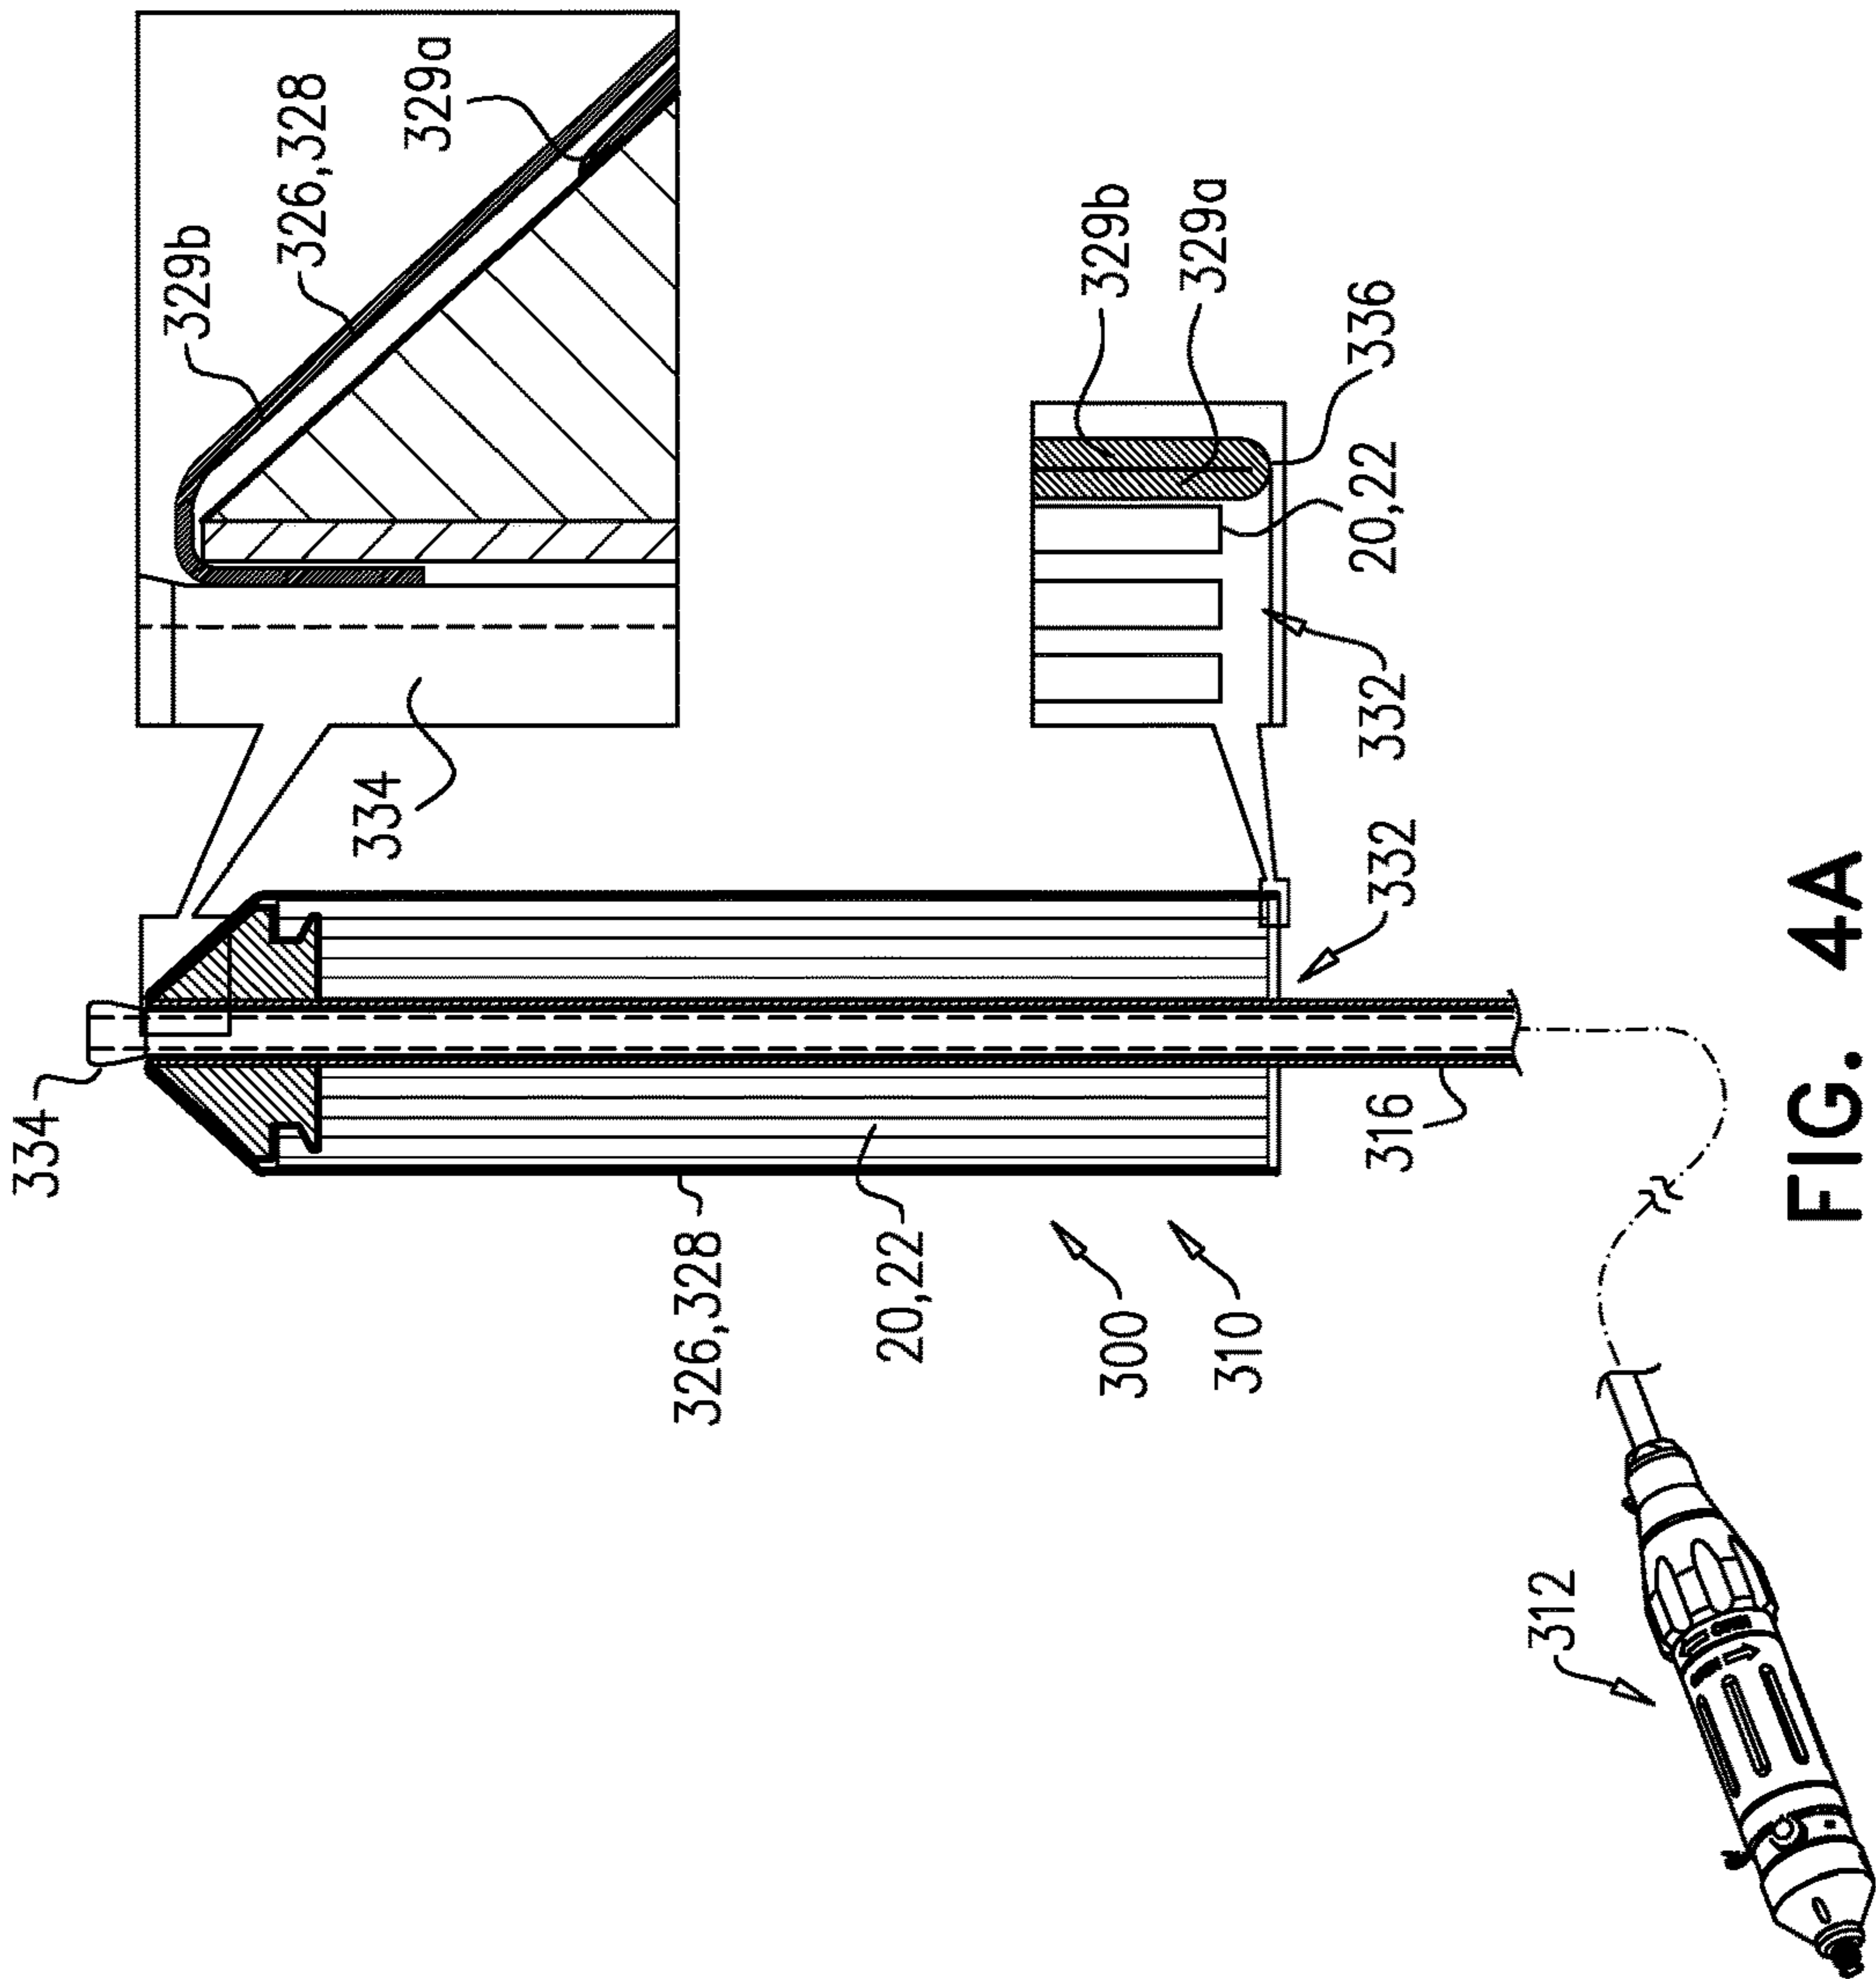


FIG. 4A

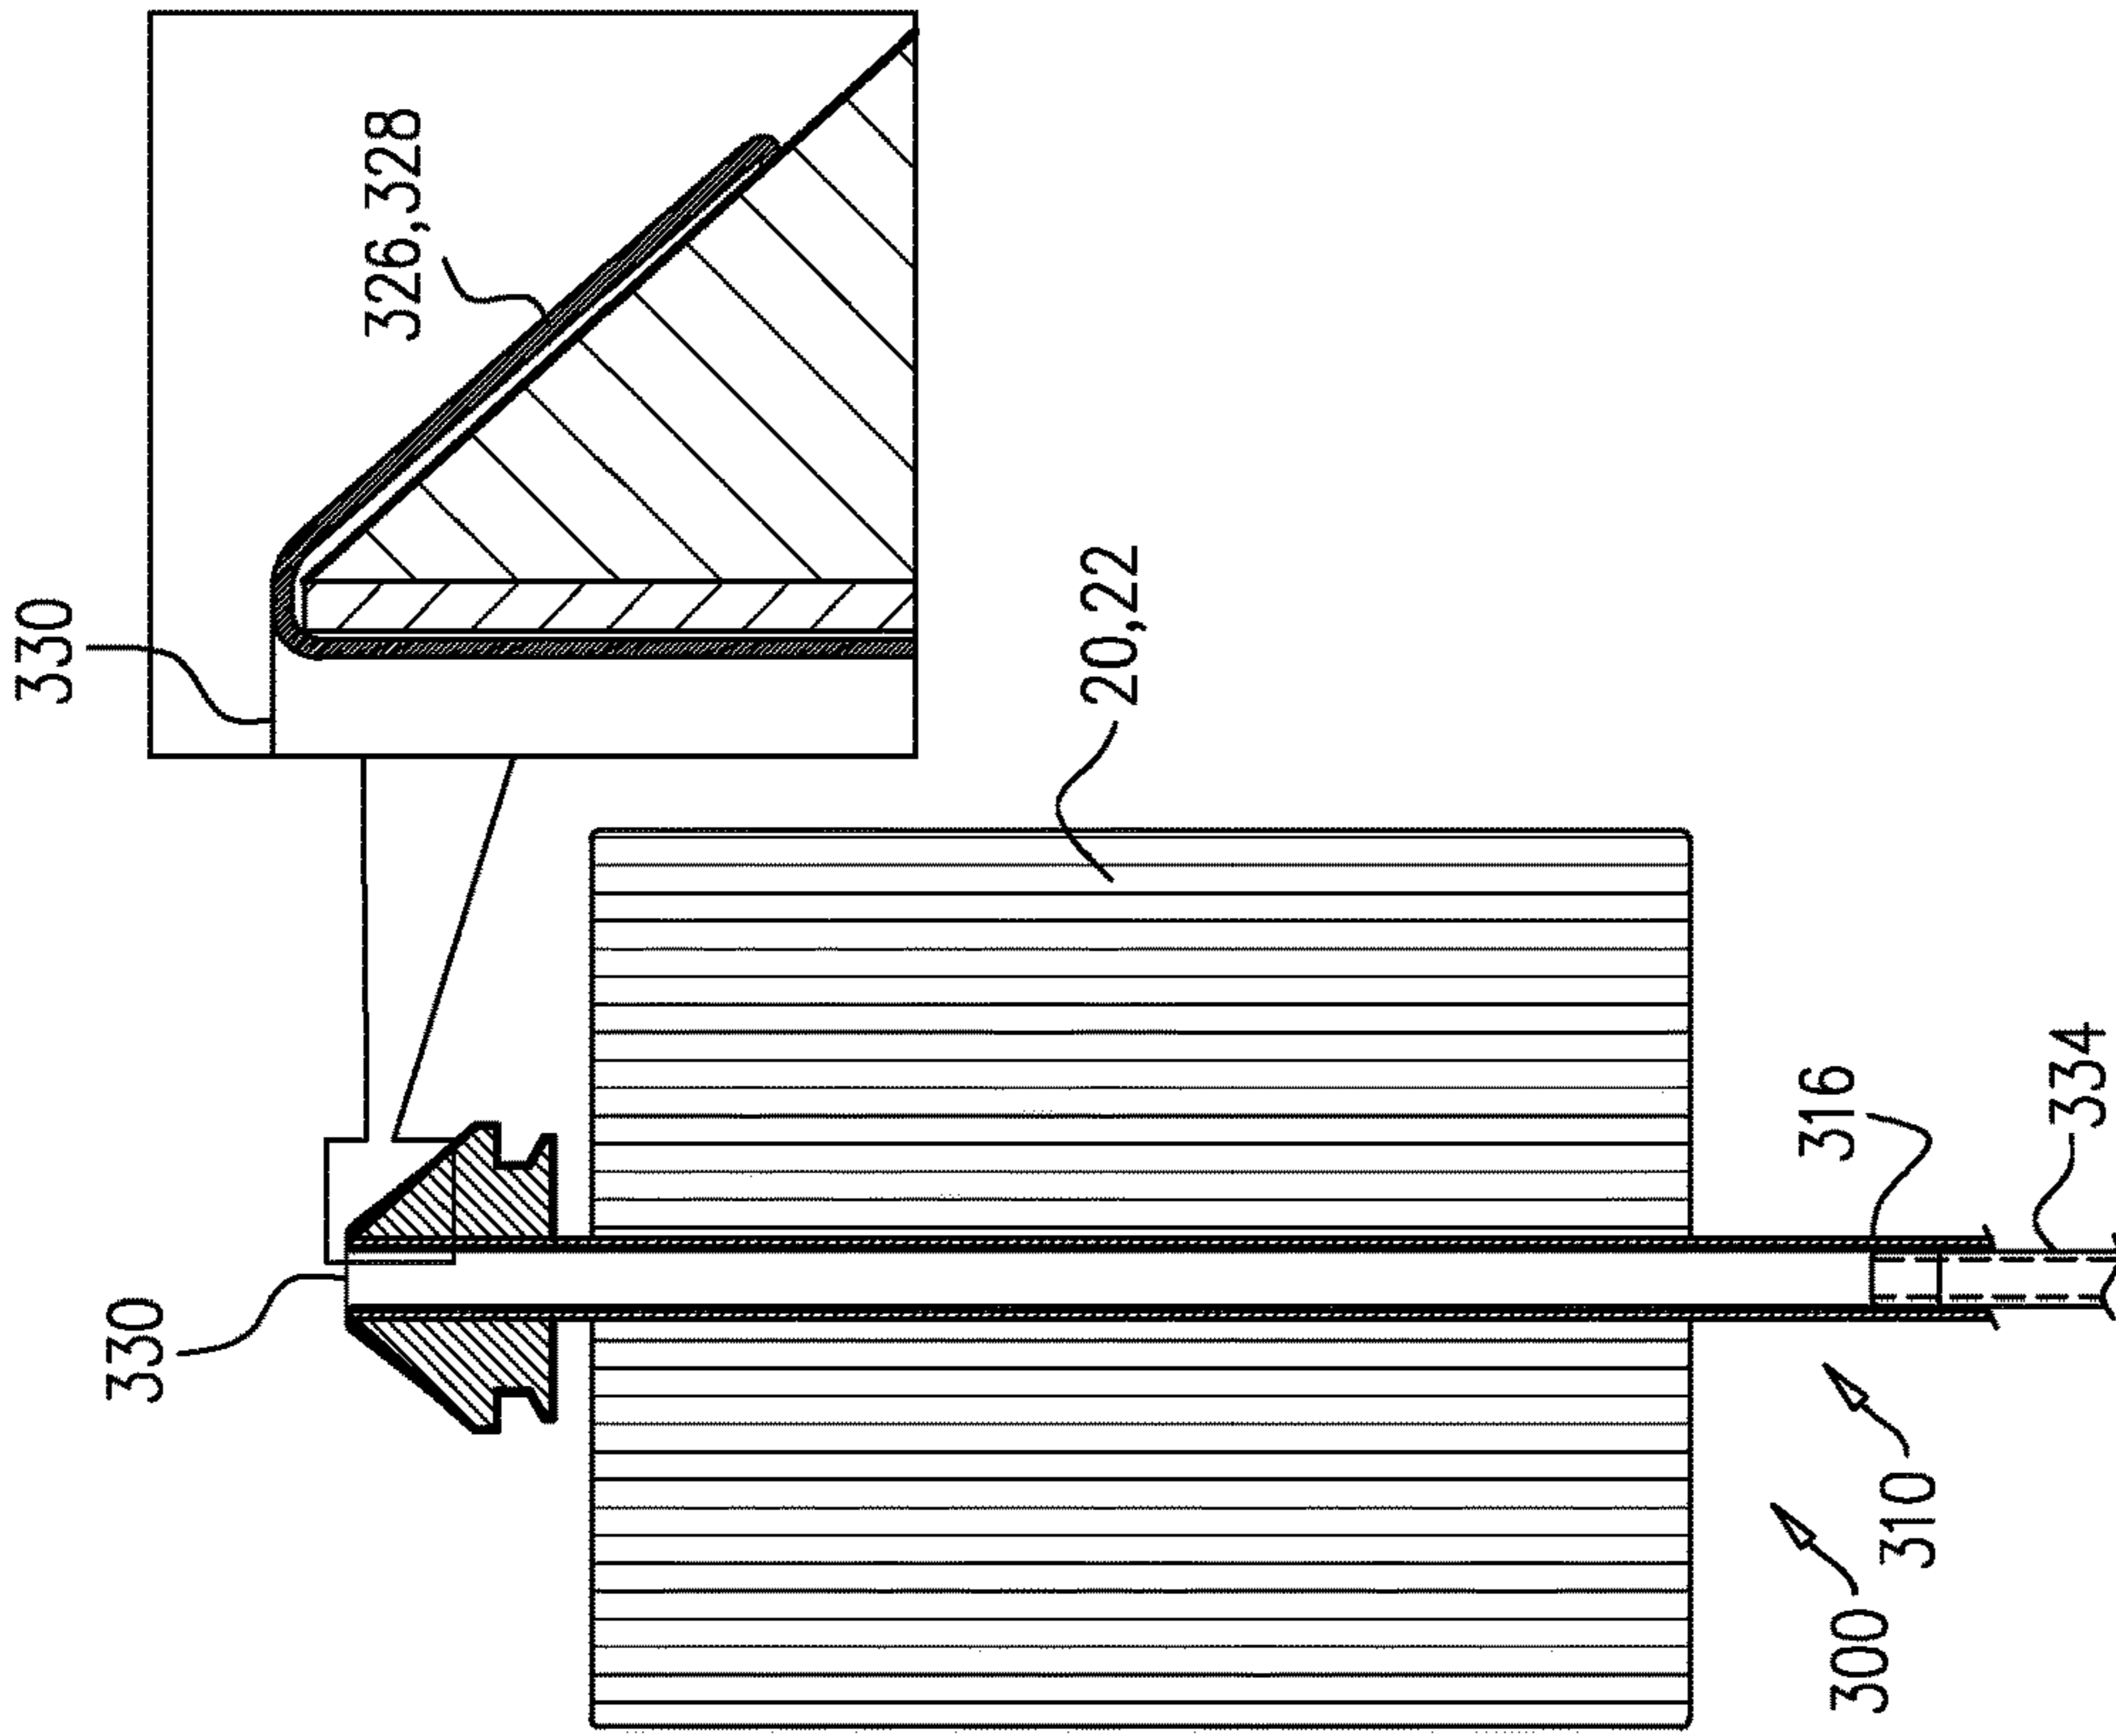


FIG. 4C

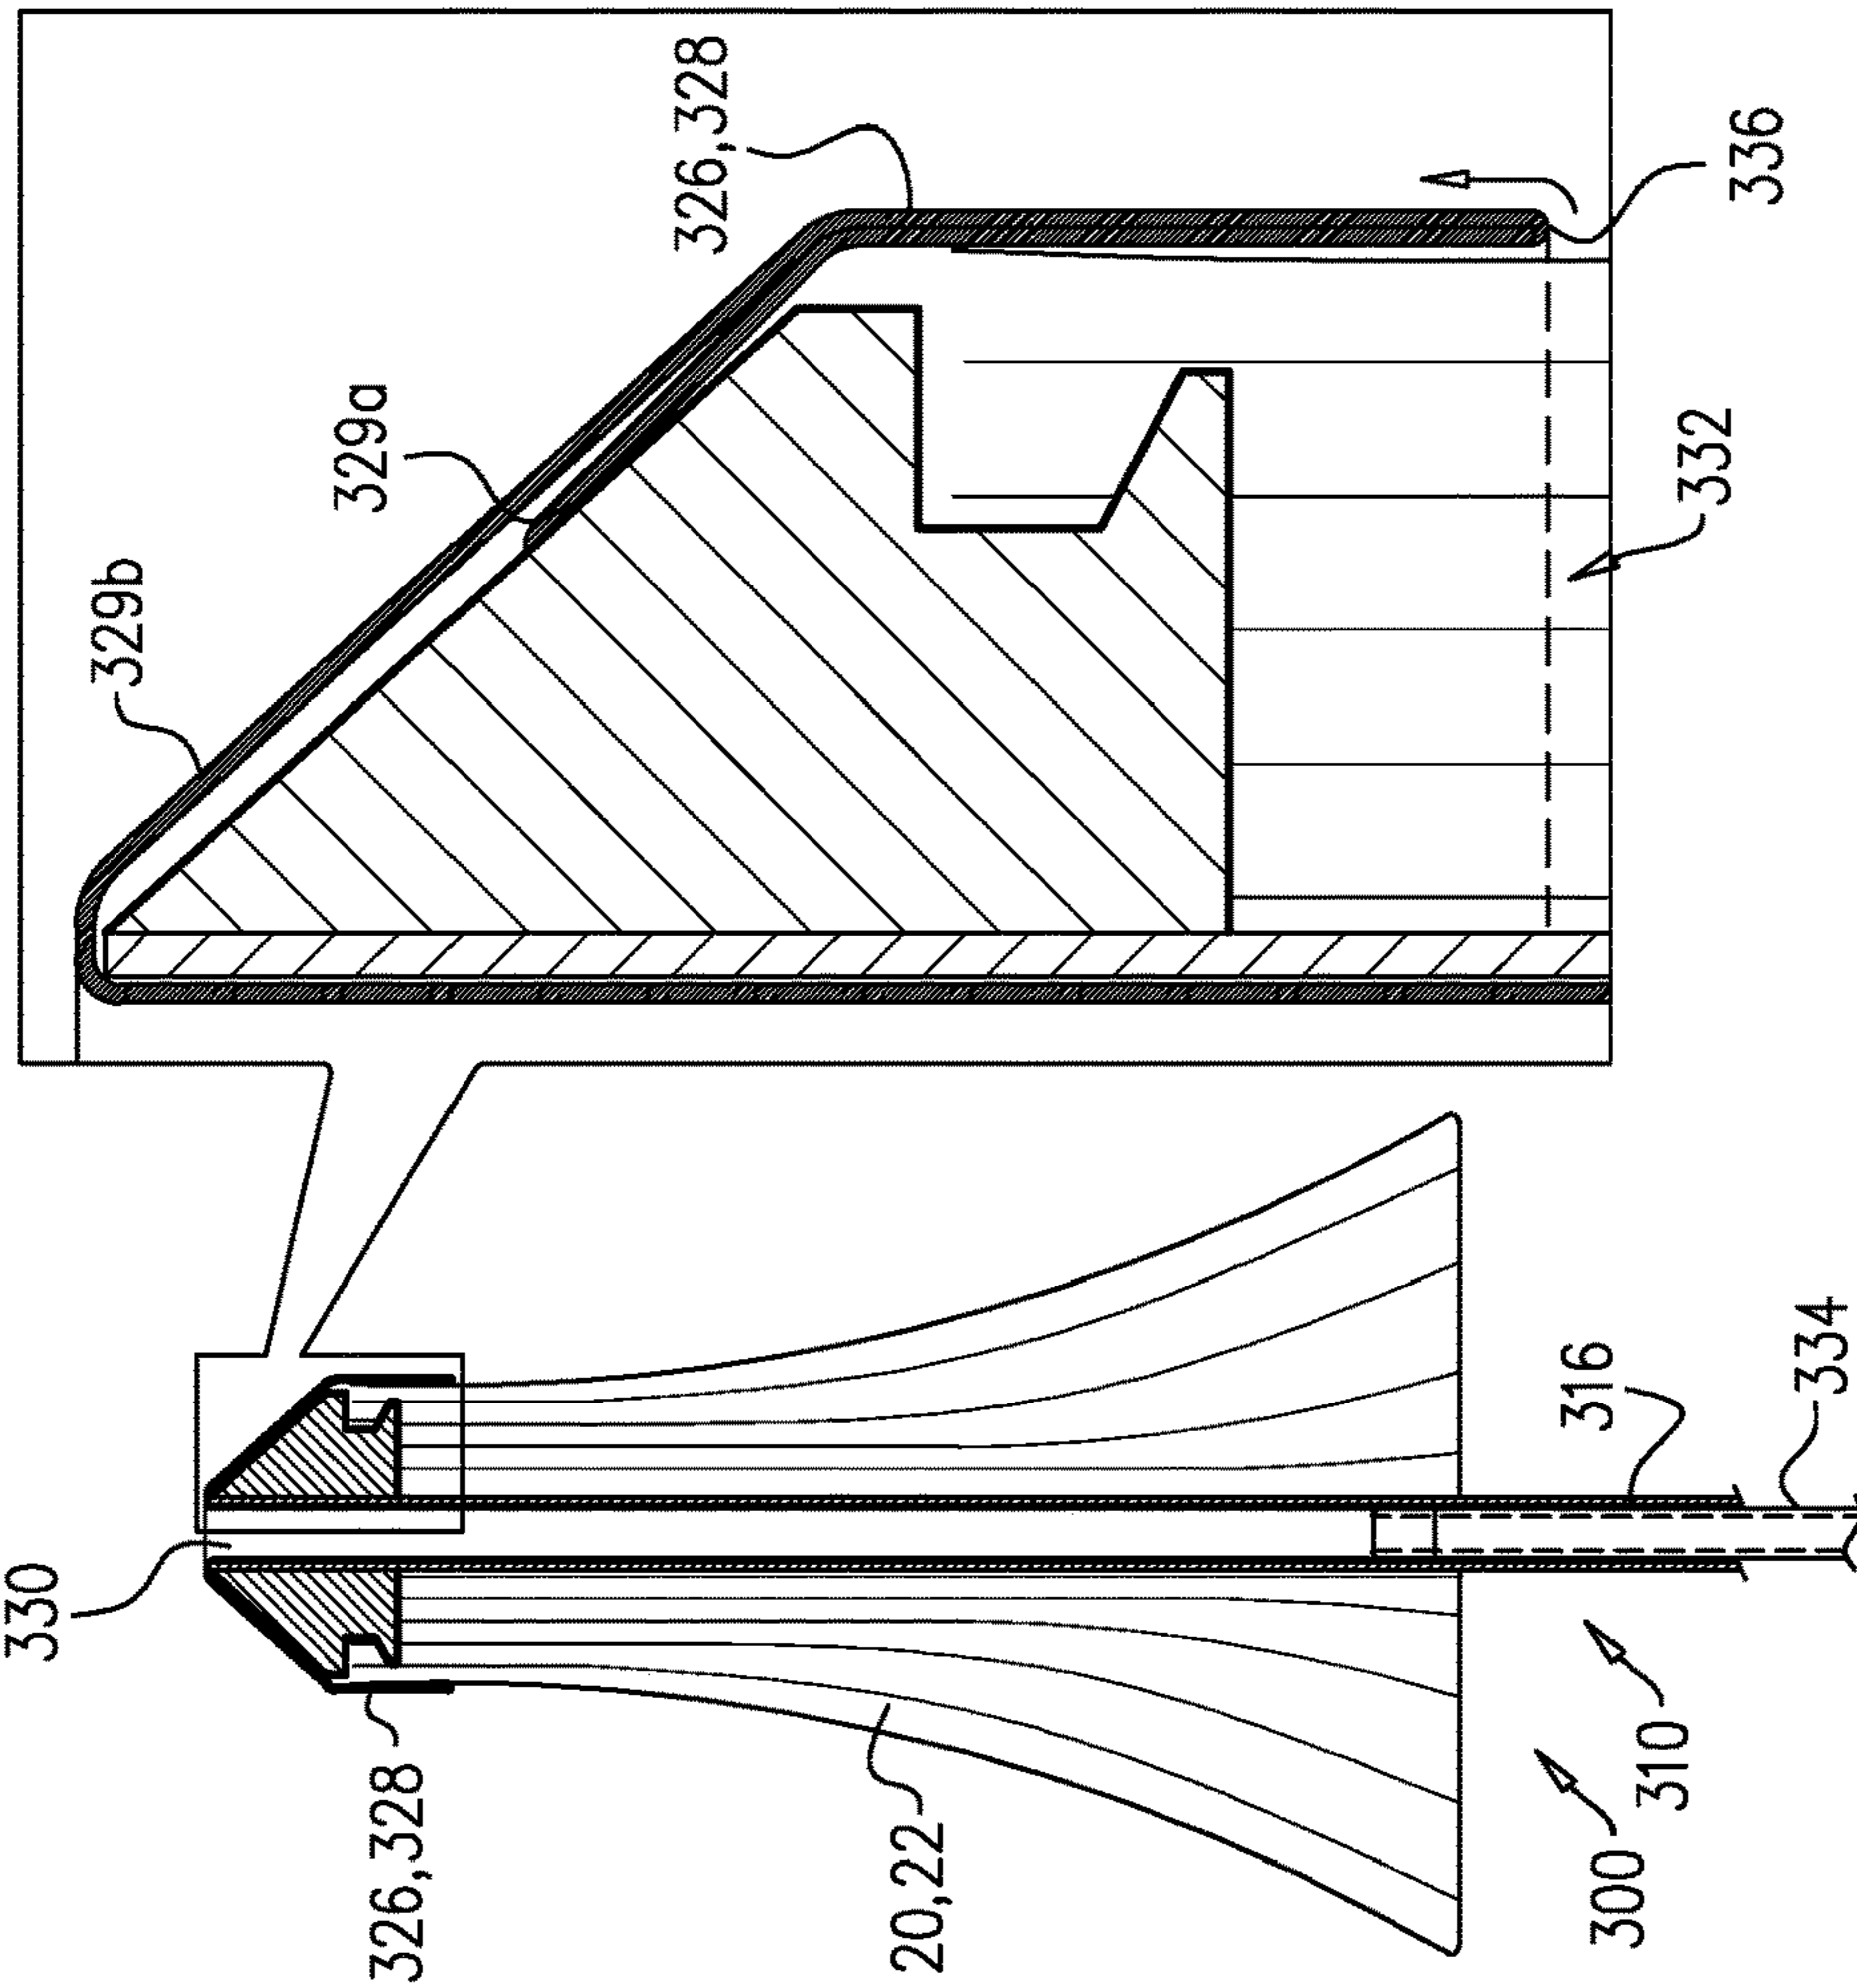


FIG. 4D



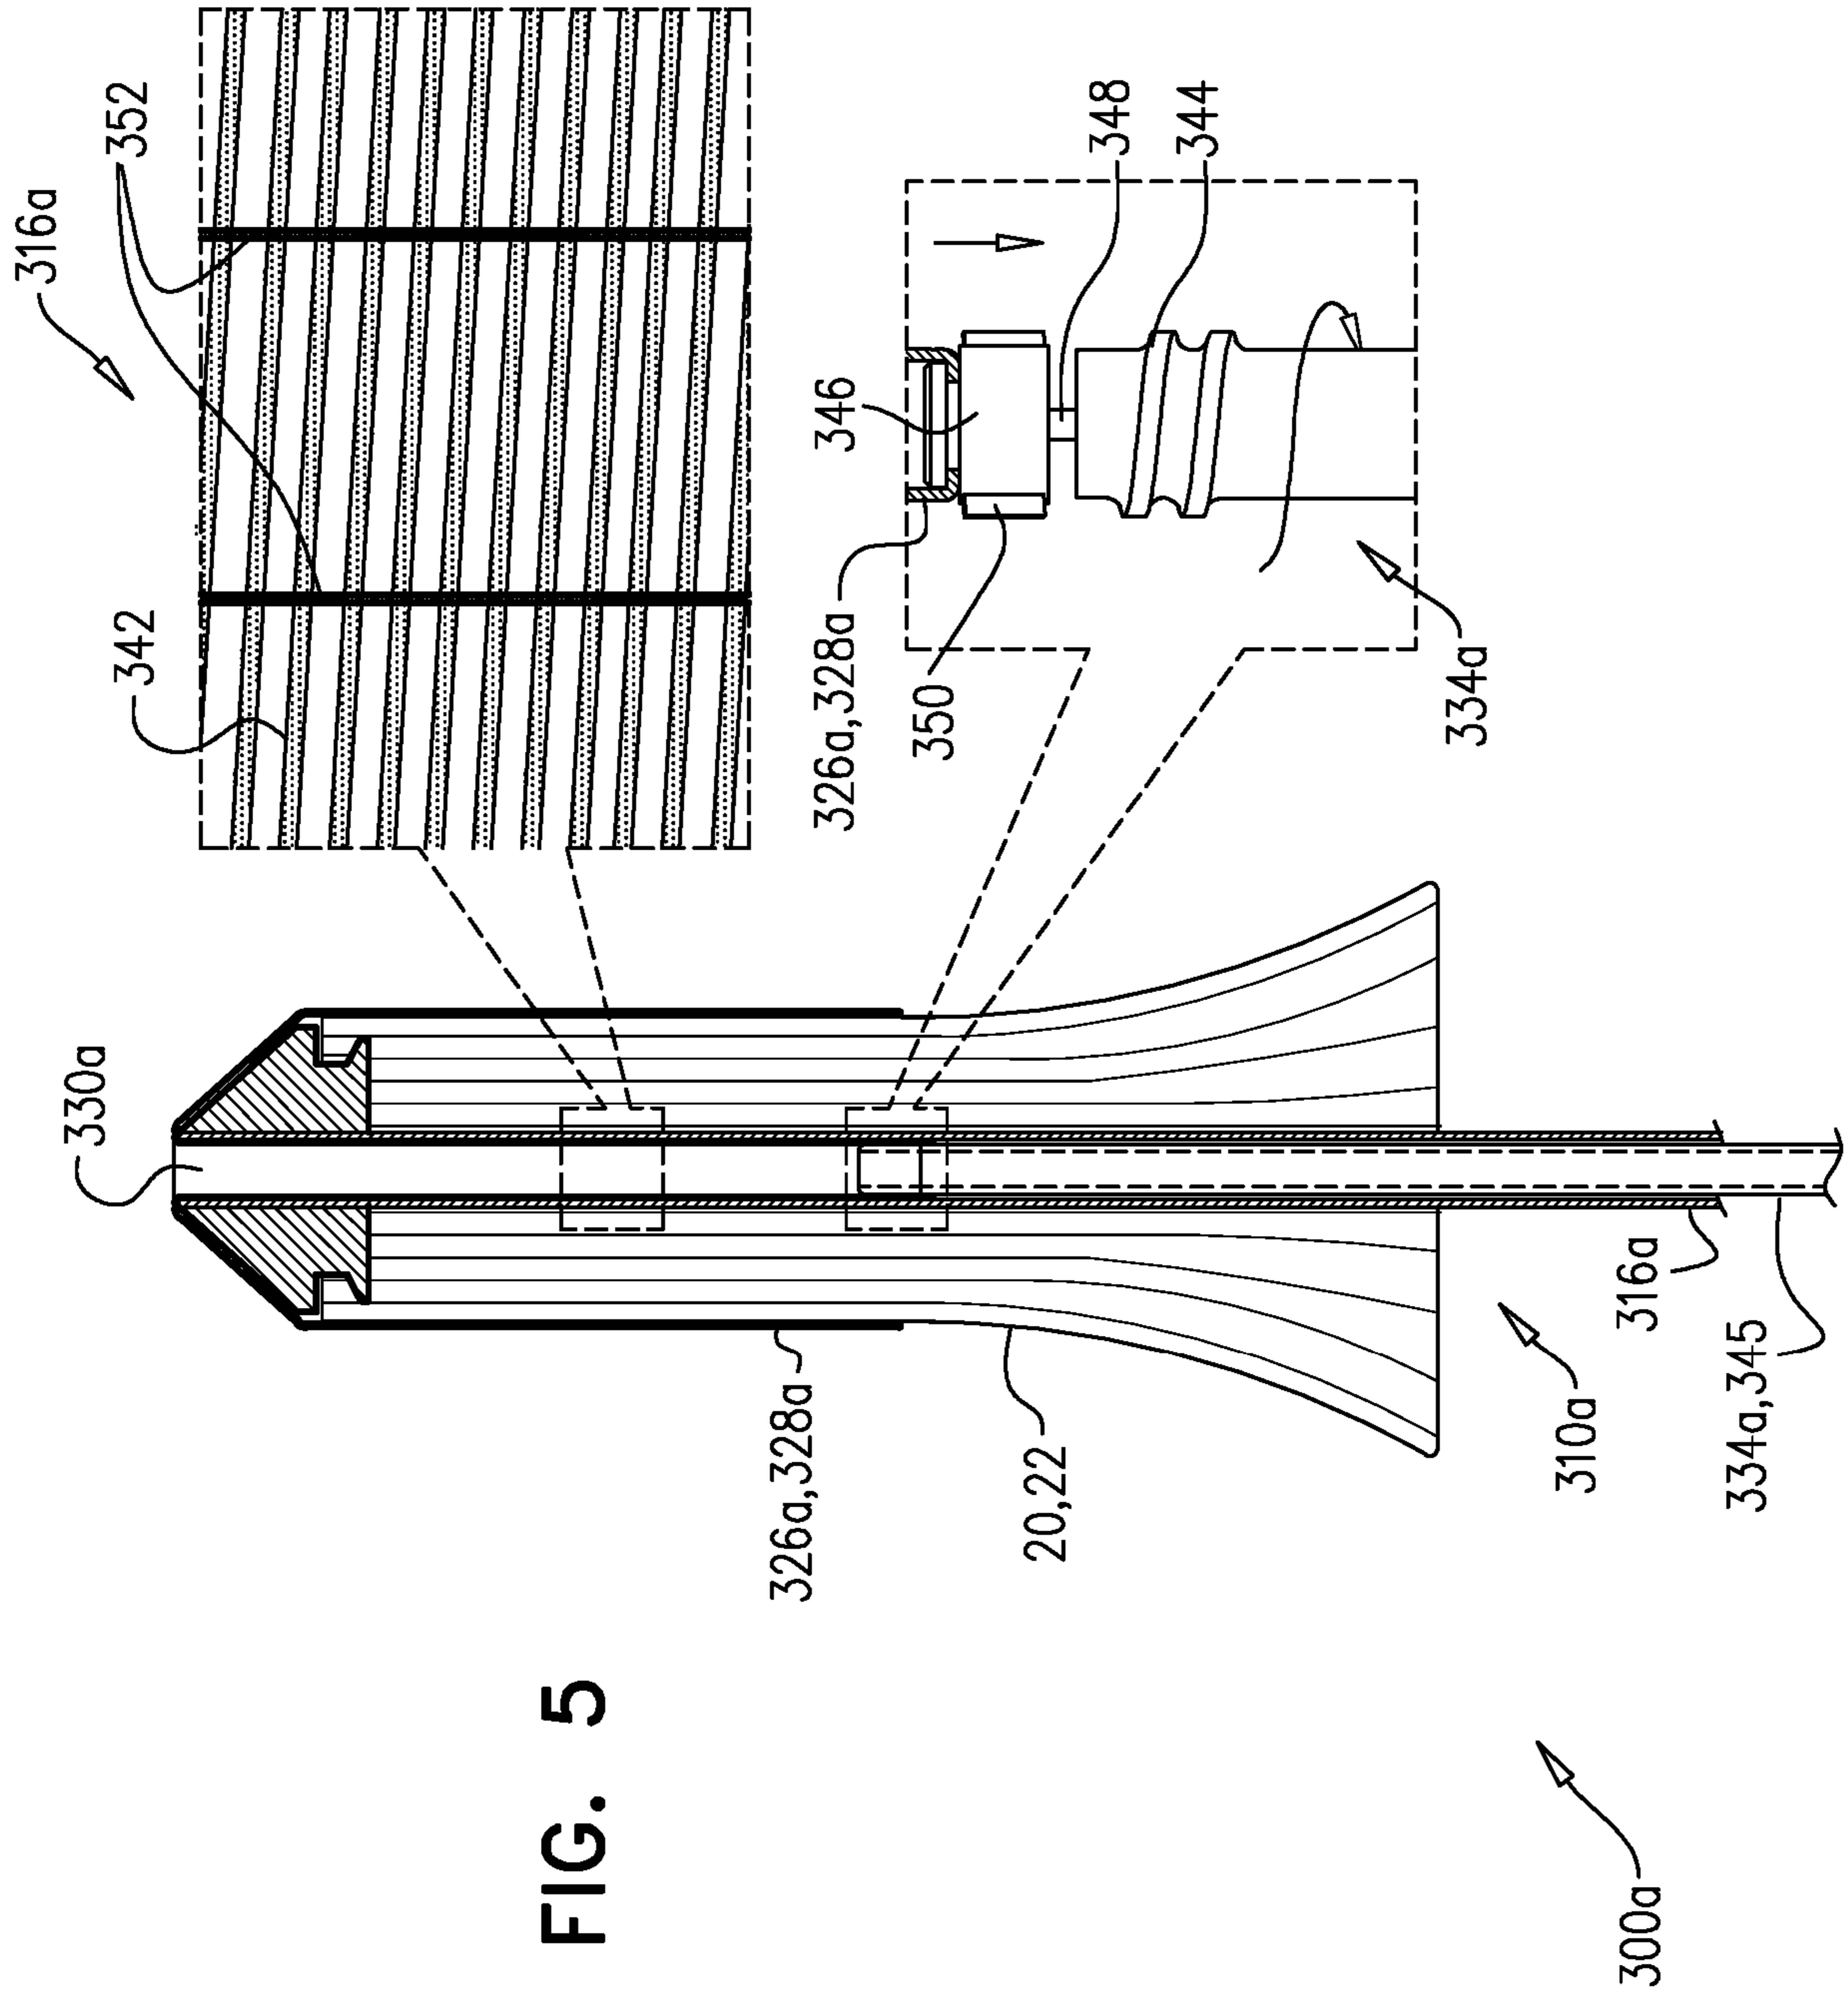


FIG. 5





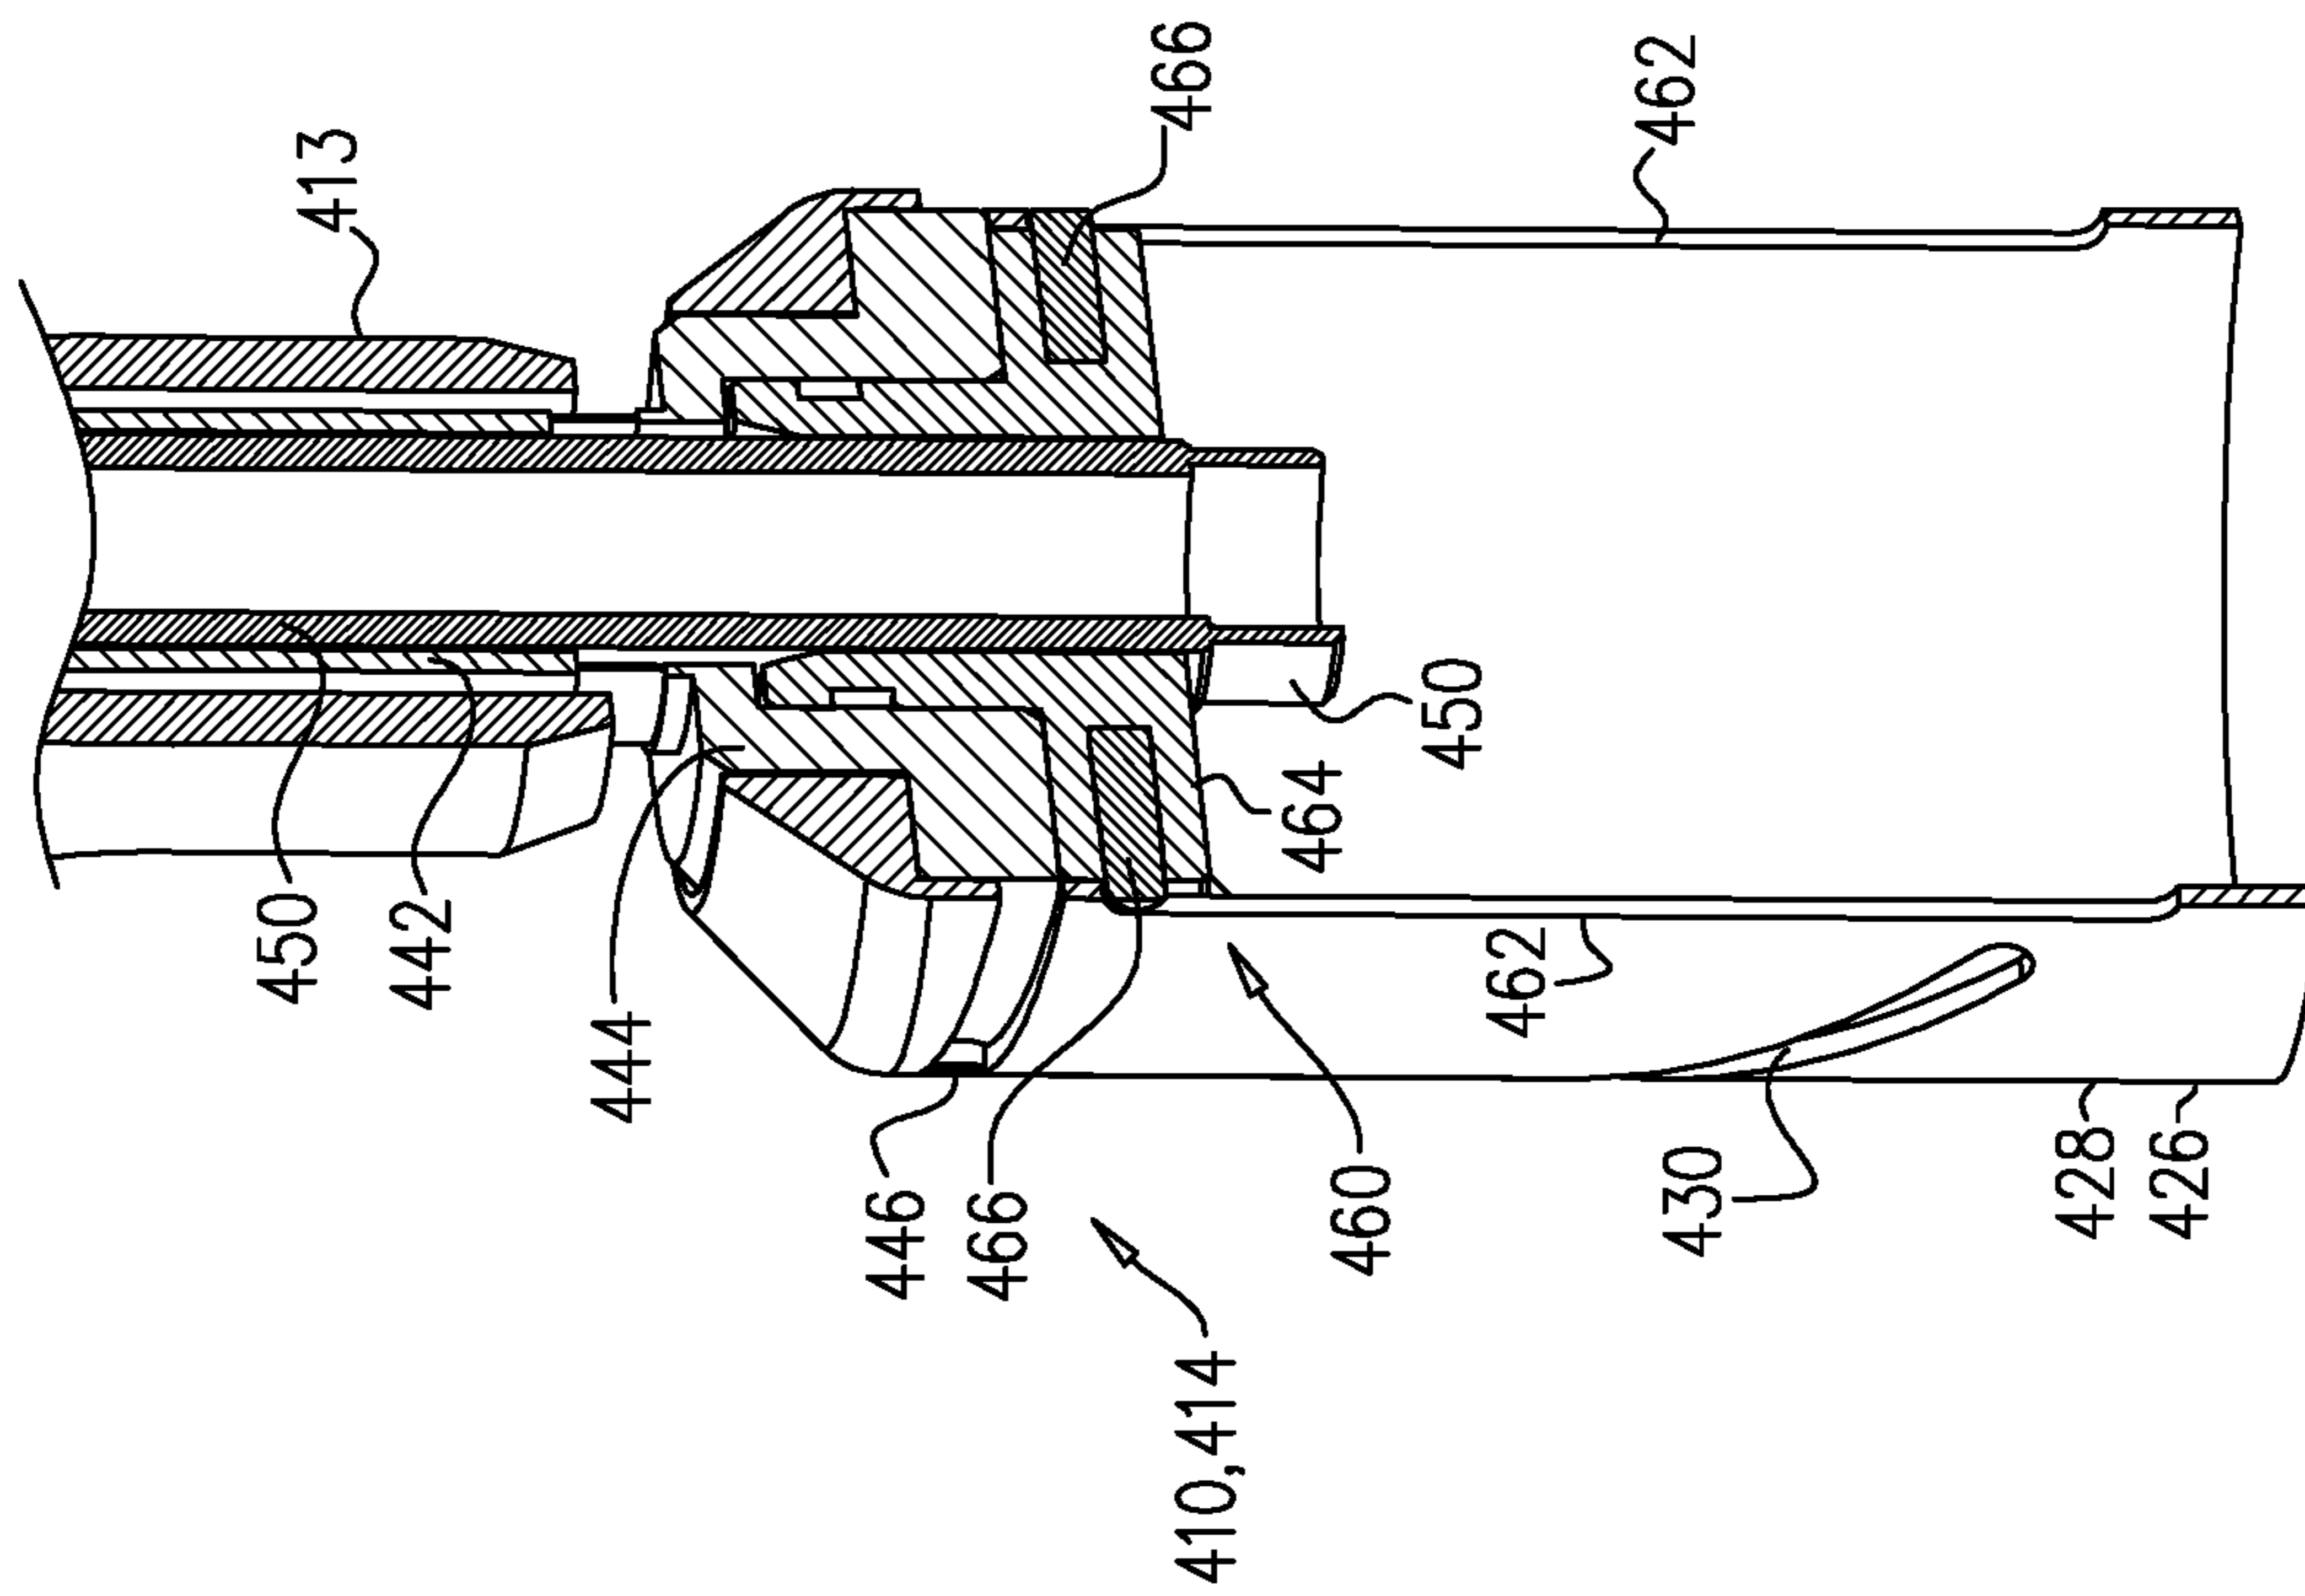


FIG. 6B

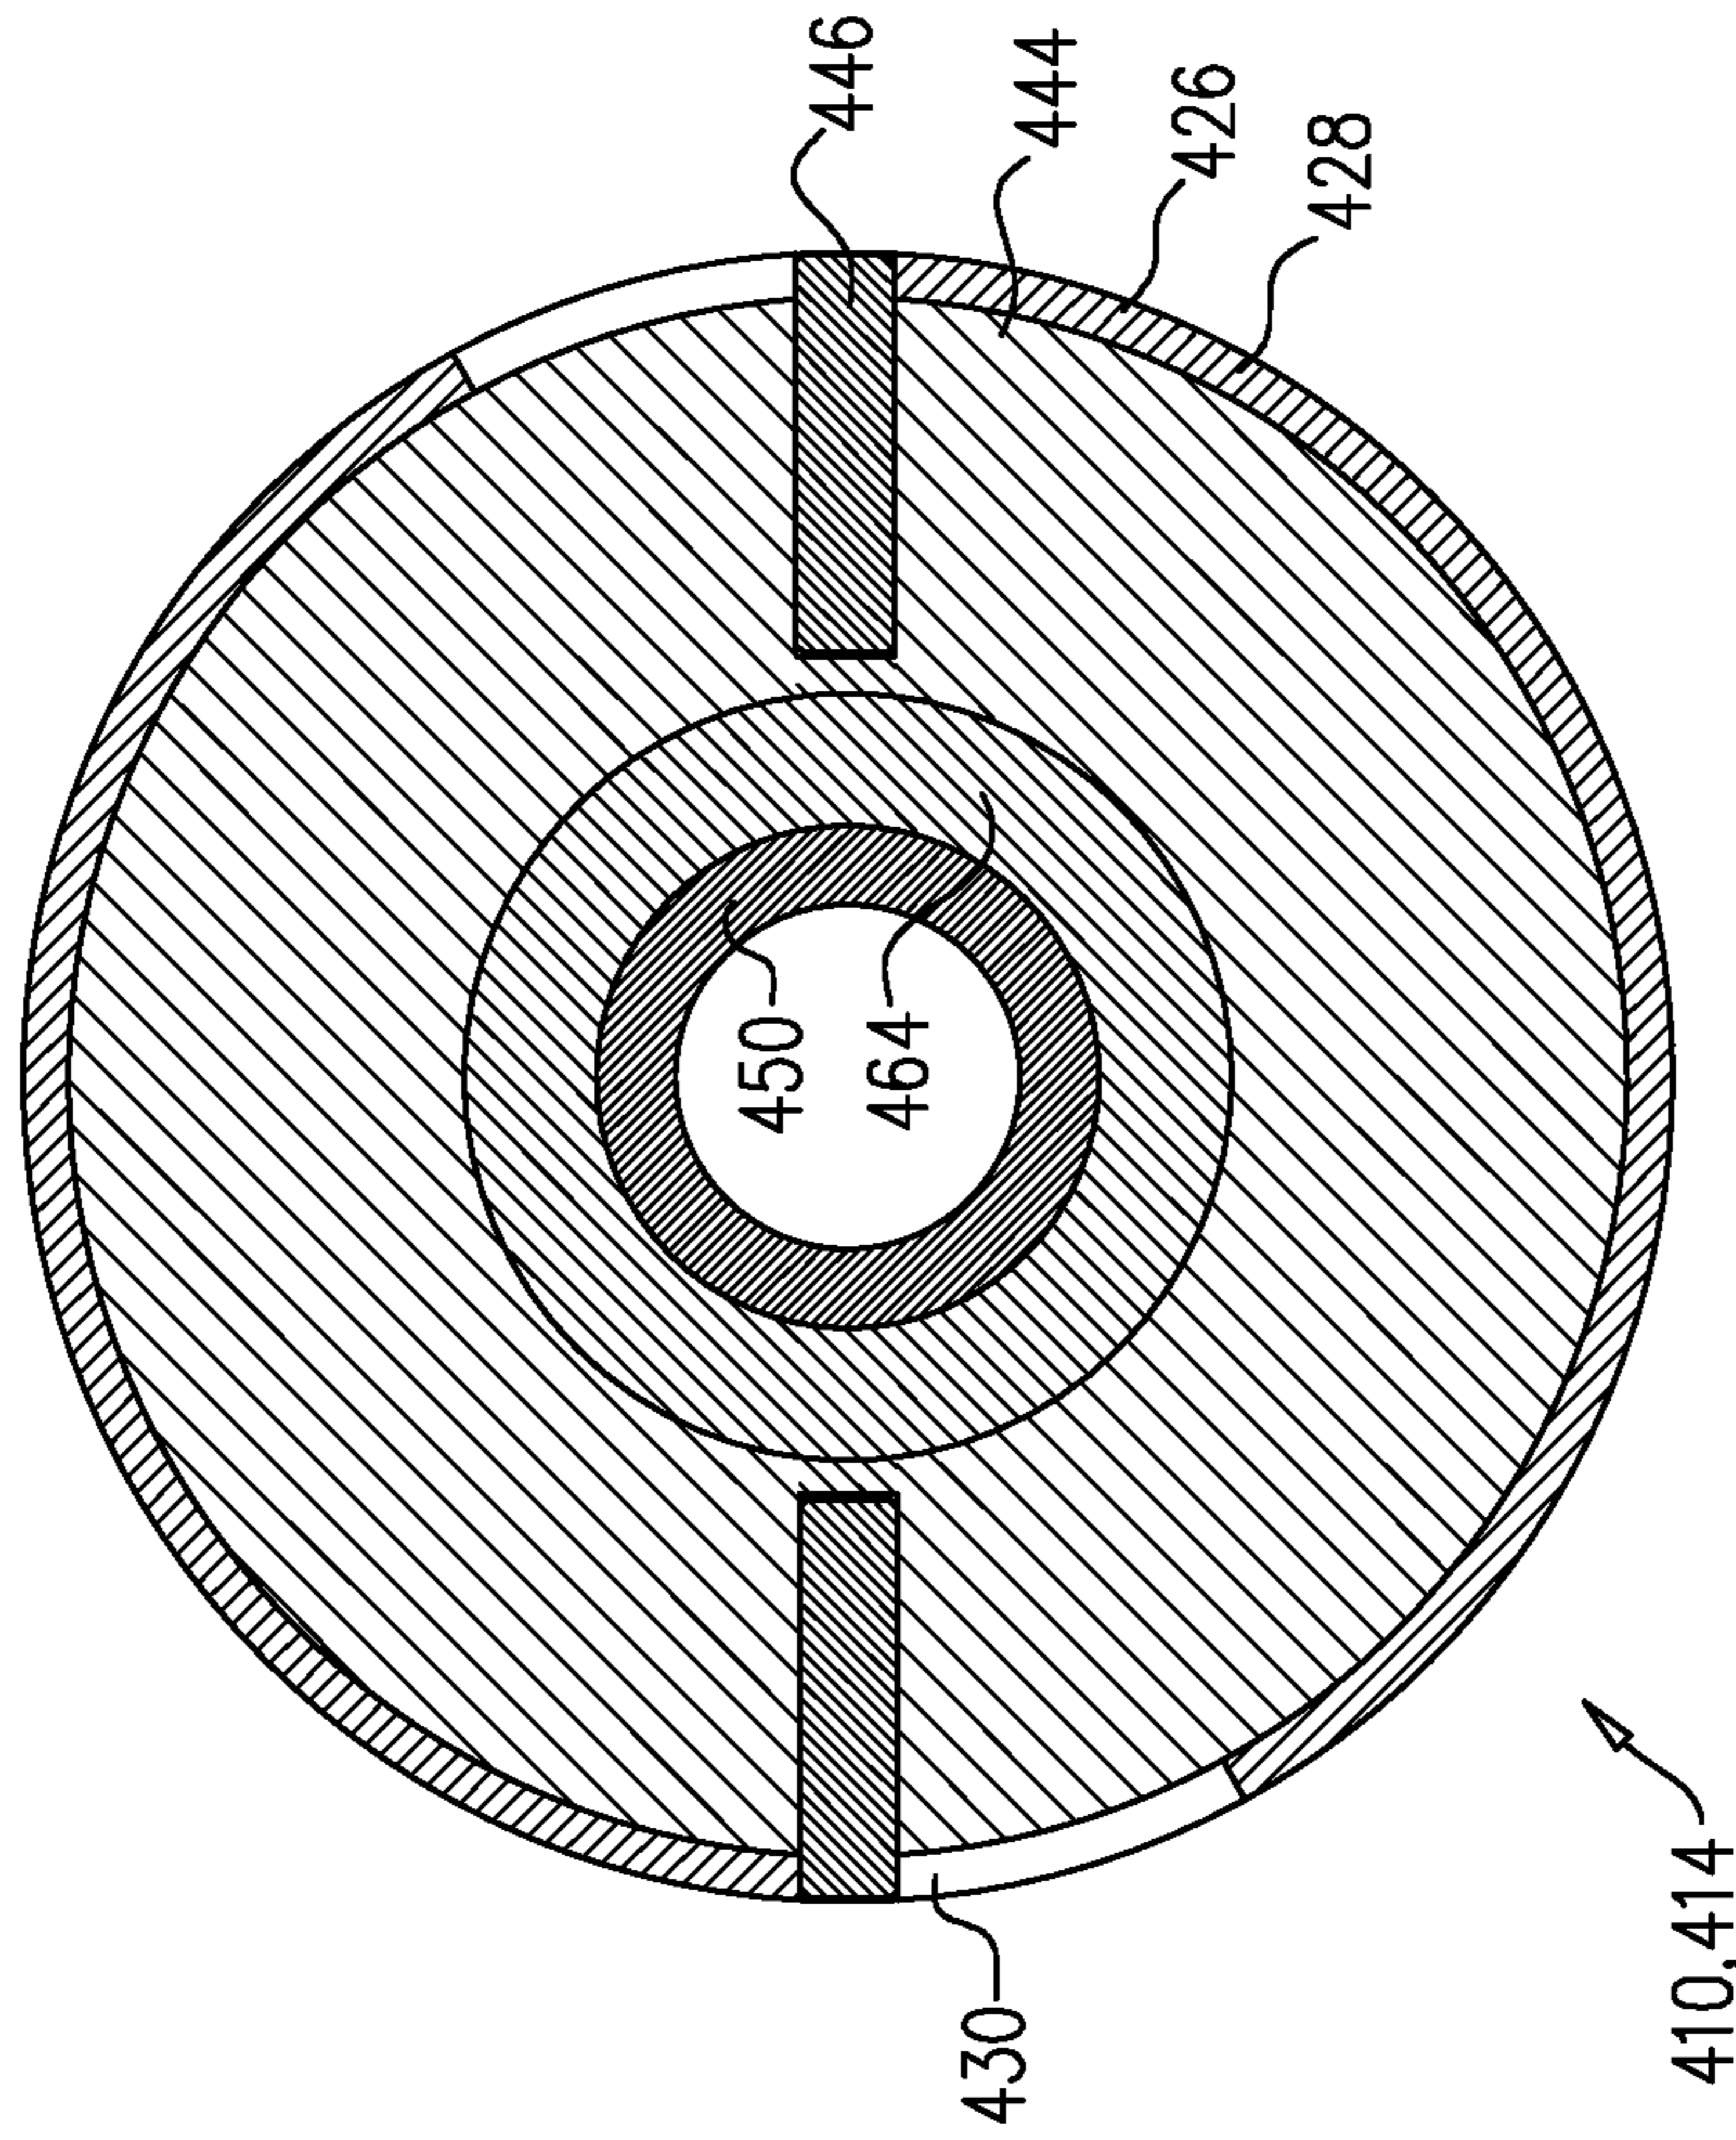
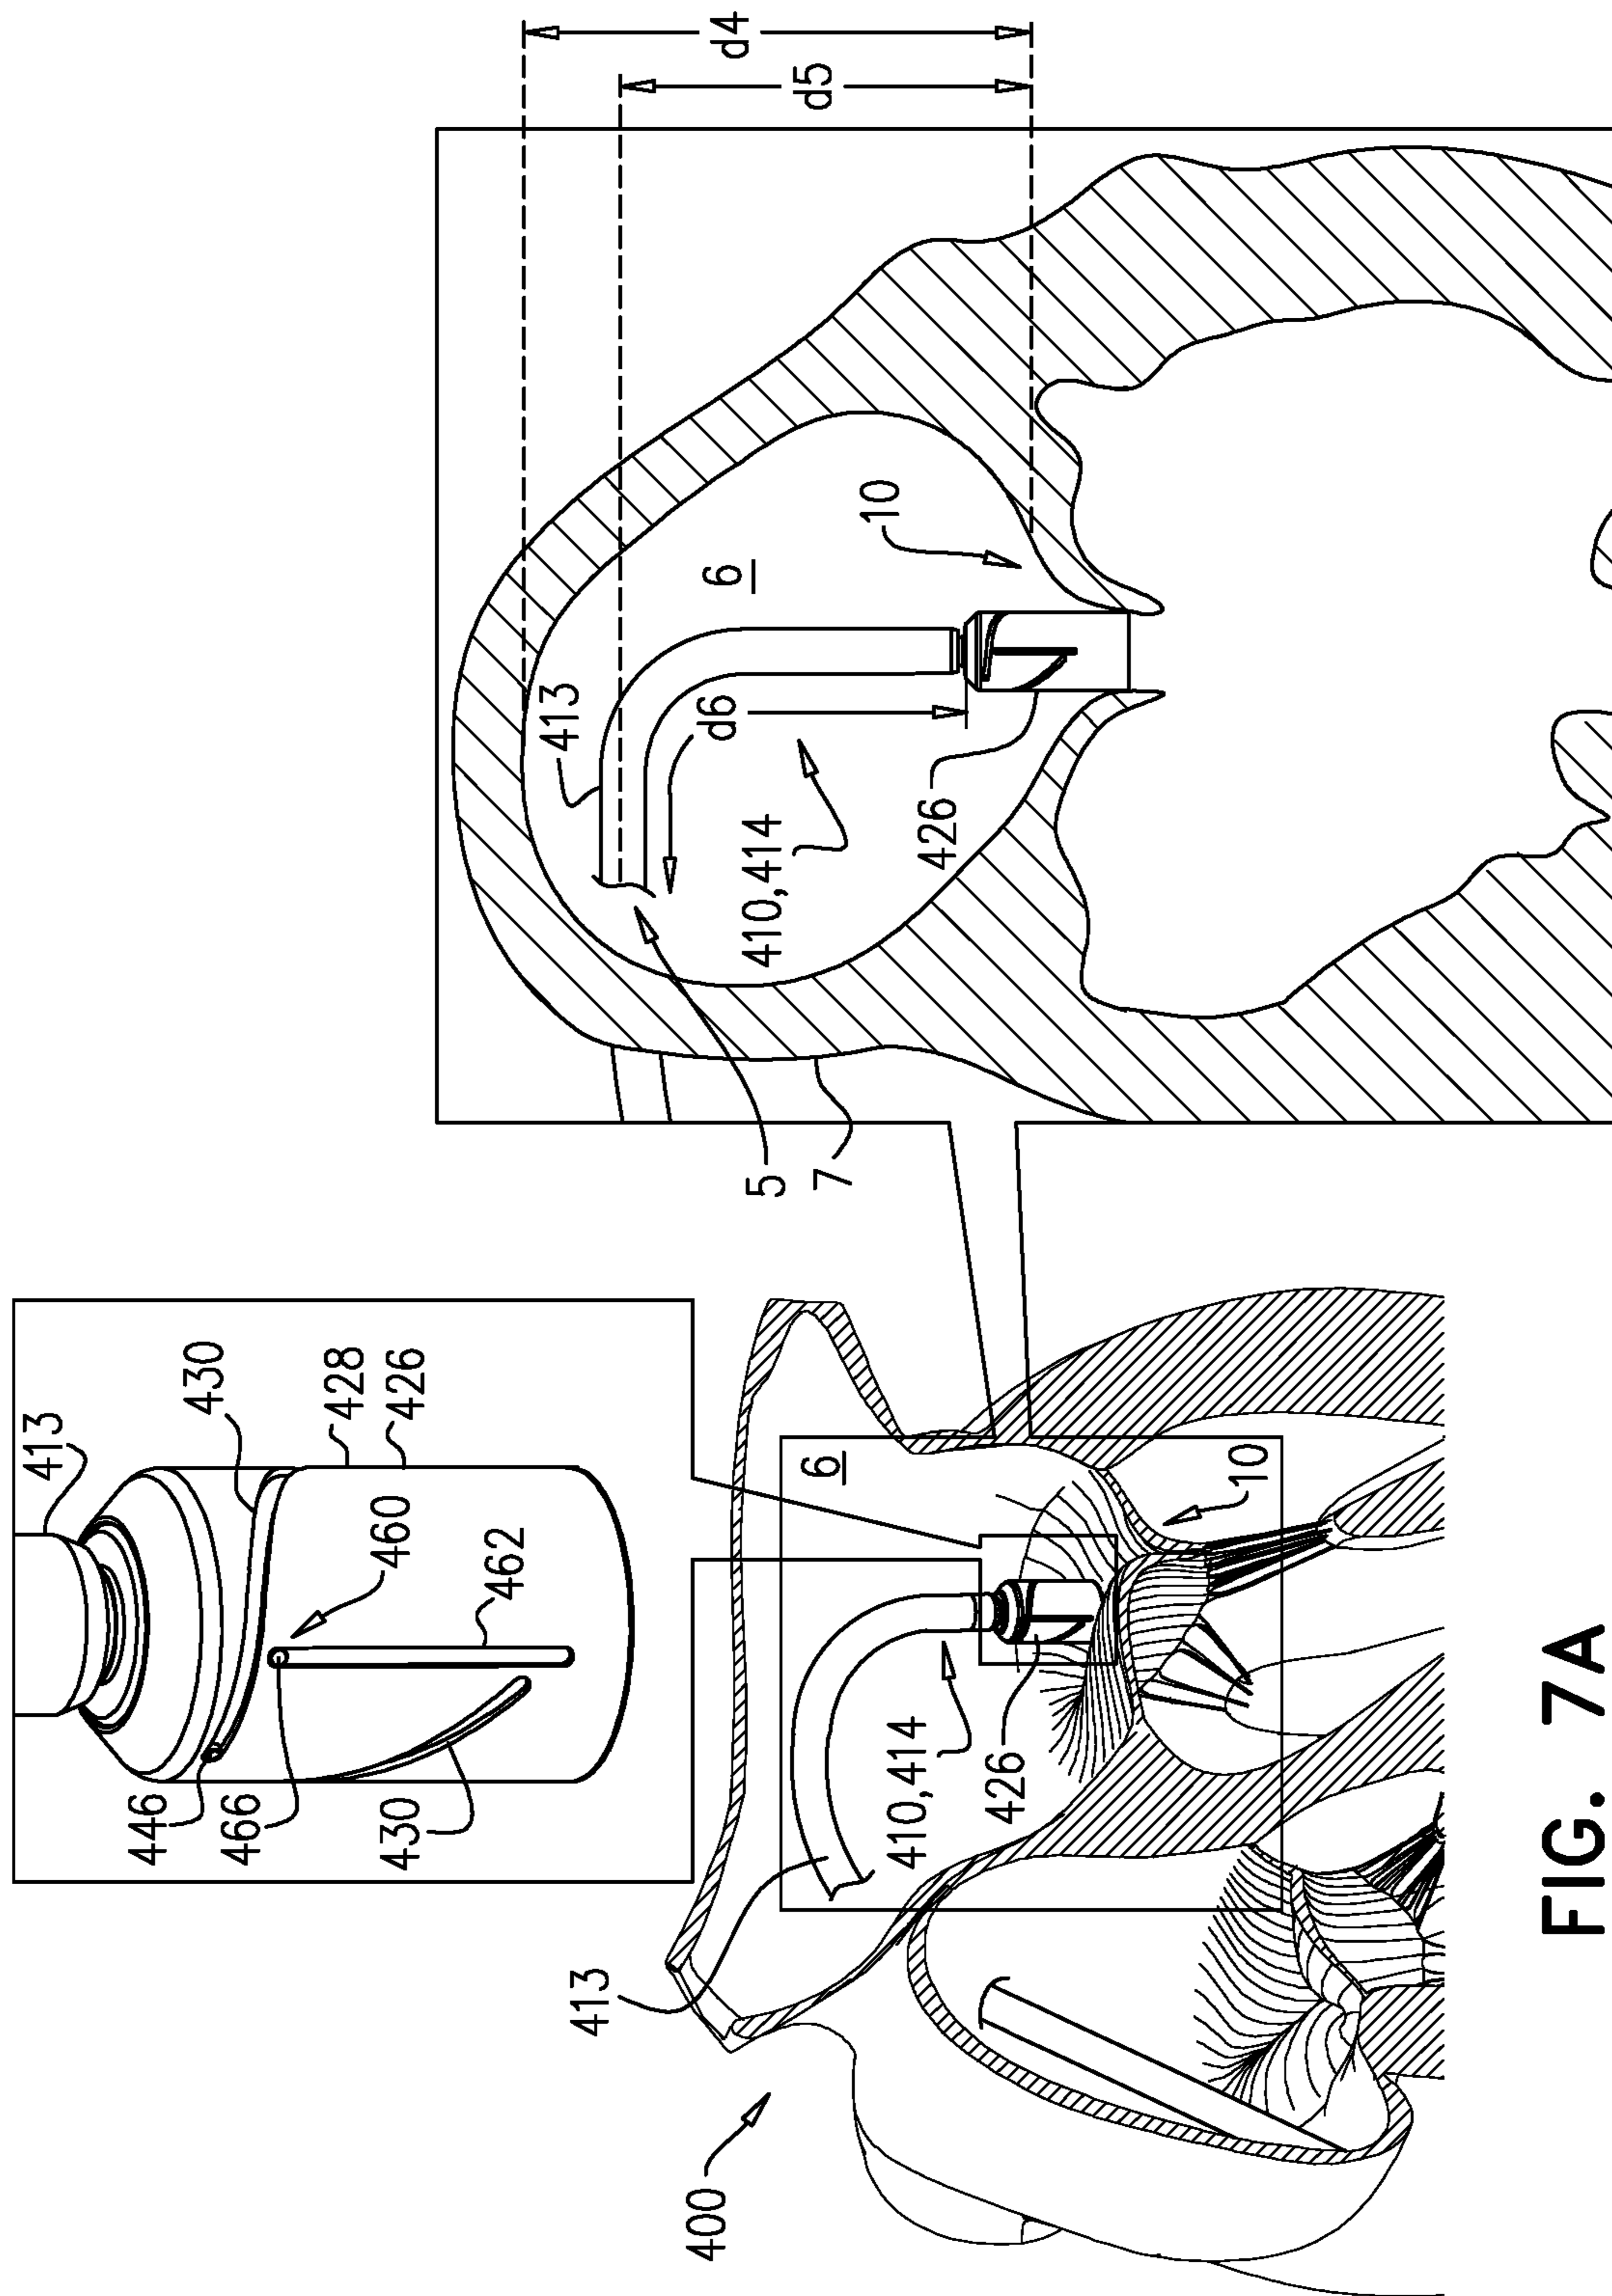


FIG. 6C





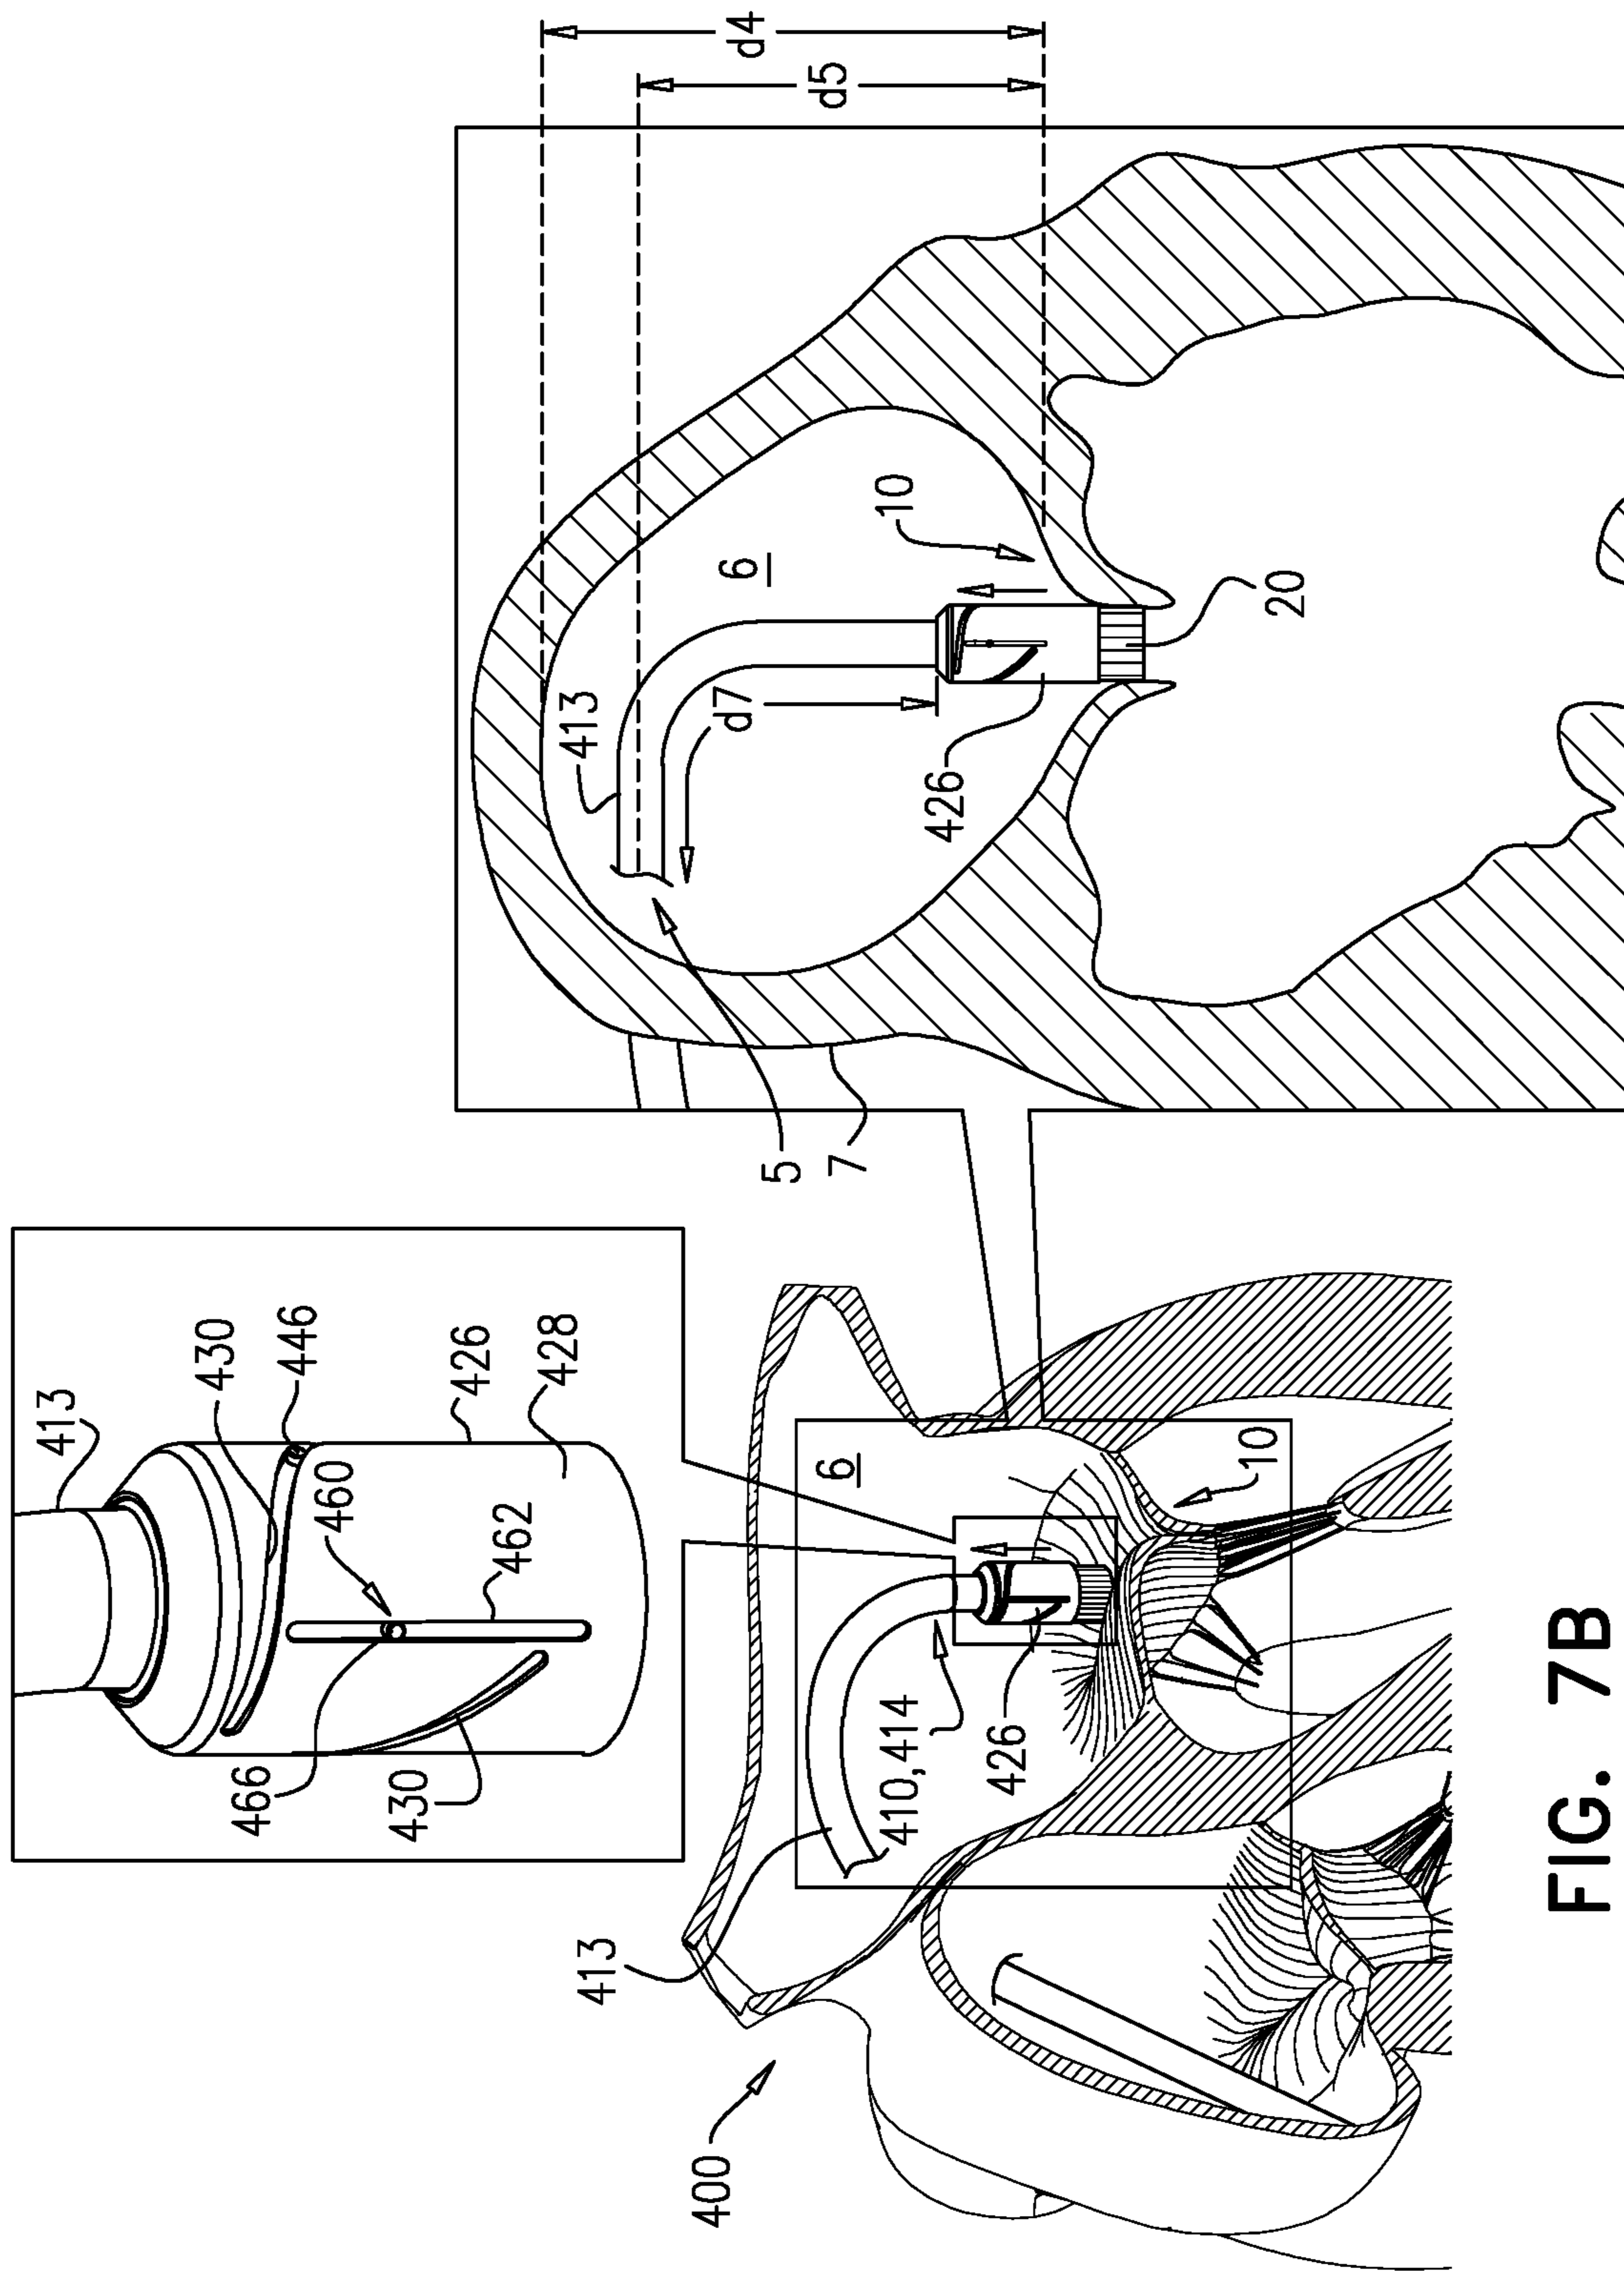


FIG. 7B

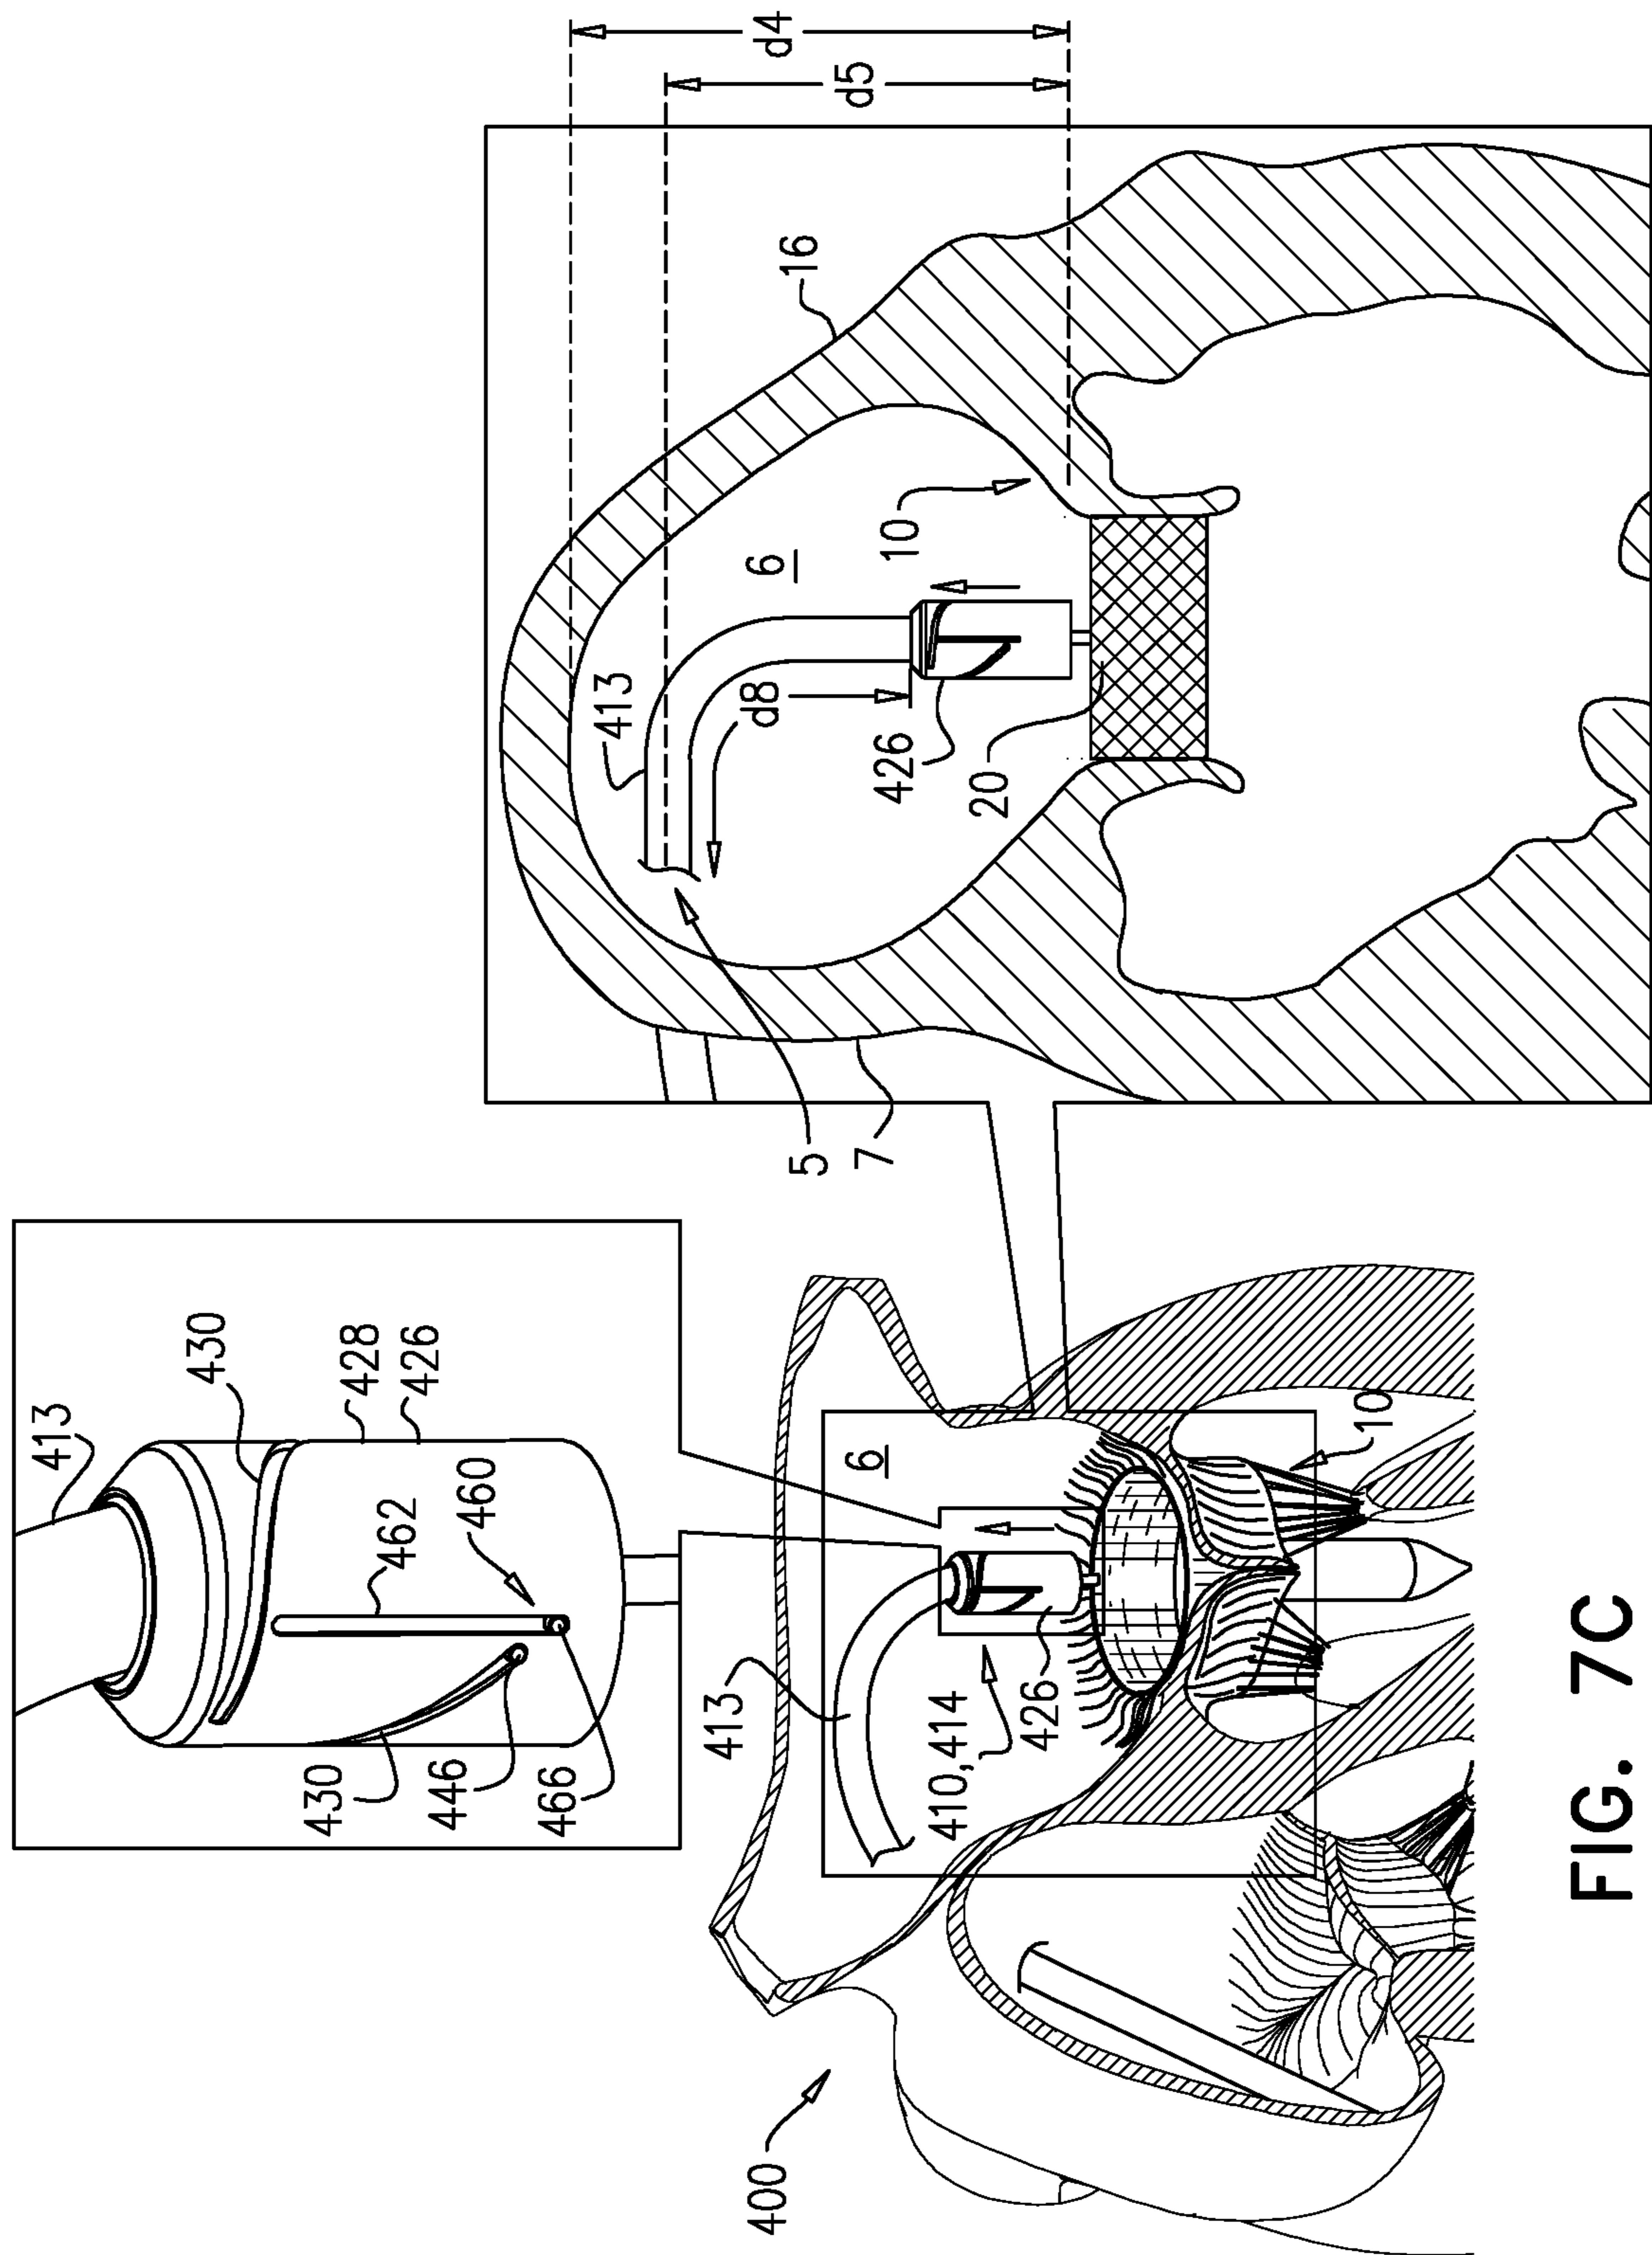


FIG. 7C



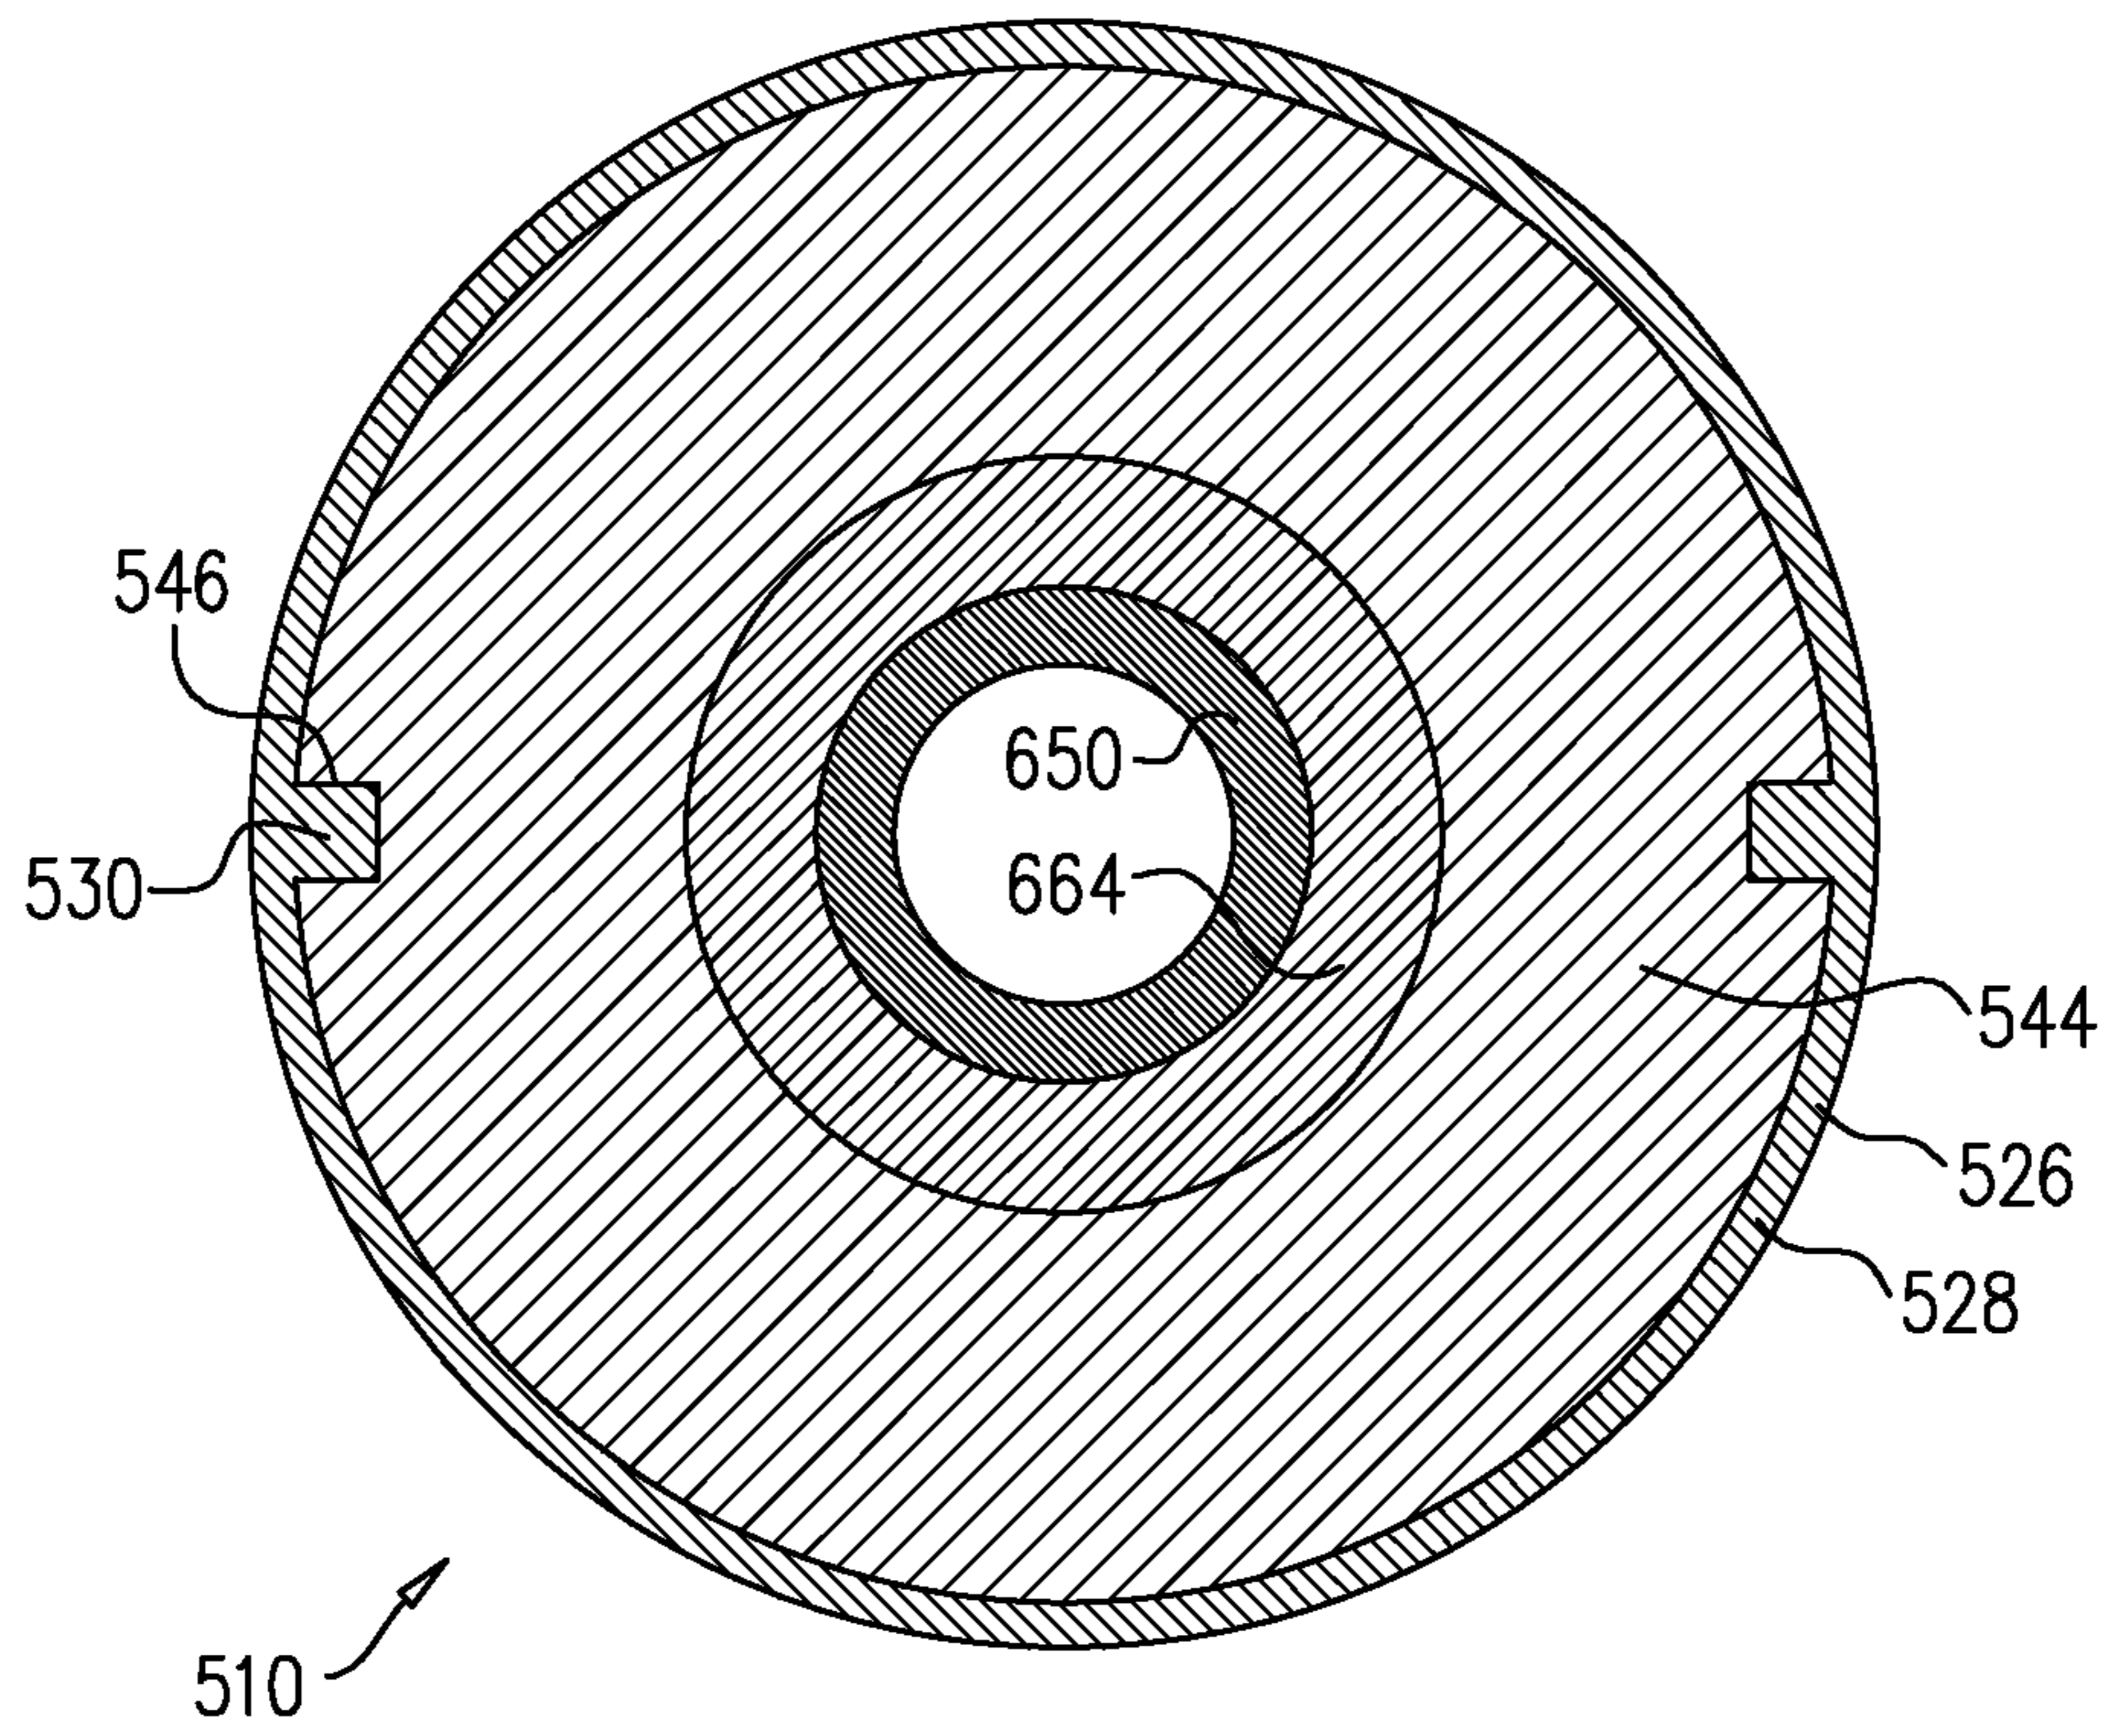


FIG. 8



## MINIMALLY-INVASIVE DELIVERY SYSTEMS

### CROSS-REFERENCES TO RELATED APPLICATIONS

The present application is the US National Phase of PCT application IL2017/050849 to Hariton et al., filed Aug. 1, 2017, and entitled "Minimally-invasive delivery systems," which claims priority from UK patent application GB1613219.3, filed Aug. 1, 2016, and entitled "Minimally-invasive delivery systems," which is incorporated herein by reference.

### FIELD OF THE INVENTION

Some applications of the present invention relate in general to valve replacement. More specifically, some applications of the present invention relate to prosthetic cardiac valves and techniques for implantation thereof.

### BACKGROUND

Dilation of the annulus of a heart valve, such as that caused by ischemic heart disease, prevents the valve leaflets from fully coapting when the valve is closed. Regurgitation of blood from the ventricle into the atrium results in increased total stroke volume and decreased cardiac output, and ultimate weakening of the ventricle secondary to a volume overload and a pressure overload of the atrium.

### SUMMARY OF THE INVENTION

Systems are described, each of which comprises a delivery tool for an implant, the delivery tool comprising a balloon at a distal portion of the tool. The balloon facilitates movement of the distal portion of the tool past potential anatomical and/or implanted obstacles, e.g., by providing a tapered surface. One described balloon serves as a nosecone of the delivery tool, facilitating distal movement of the distal portion of the tool through the vasculature. Another described balloon serves as a reverse nosecone that facilitates proximal movement of the distal portion of the tool through the implanted implant.

Also described is a sheath for retaining the implant on the distal portion of a delivery tool, and a system for unsheathing the implant.

Also described is a delivery tool that comprises a housing that defines a generally-helical track, and a controller that comprises an actuator. At least part of an implant is housed by the housing. Rotation of the actuator draws the housing proximally with respect to the implant by sliding an engaging element of the actuator along the track. This proximal movement of the housing deploys the implant from within the housing.

The technologies described may be used separately on different delivery tools, or in various combinations on a single delivery tool.

There is therefore provided, in accordance with an application of the present invention, apparatus, for use with an implant, the apparatus including a tool, the tool including:

- a housing, at a distal part of the tool, the housing:
  - including a tubular wall that circumscribes a longitudinal axis of the distal part of the tool, dimensioned to house at least part of the implant, and defining a track that follows a generally-helical path around the longitudinal axis; and

a controller, including:

- a rod that extends from a proximal part of the tool to the housing; and

- an actuator, fixedly coupled to the rod, including an engaging element that engages the track, and rotatable with respect to the housing, the controller and the housing mechanically cooperating such that rotation of the actuator with respect to the housing slides the housing longitudinally with respect to the actuator.

In an application:

- the housing is a proximal housing, and the part of the implant is a first part of the implant;

- the proximal housing is configured to house the first part of the implant, and has a distal opening for deployment of the first part of the implant therethrough; and

- the tool further includes a distal housing that is configured to house a second part of the implant, and has a proximal opening for deployment of the second part of the implant therethrough, the proximal opening of the distal housing facing the distal opening of the proximal housing.

In an application, the housing is dimensioned to house at least the part of the implant such that at least the part of the implant is coincident along the longitudinal axis with at least part of the track.

In an application, the housing is dimensioned to house at least the part of the implant such that the generally-helical path around the longitudinal axis is also around at least the part of the implant, and at least part of the track follows the generally-helical path around the longitudinal axis and at least the part of the implant.

In an application:

- the tool further includes a catheter,

- the rod extends through the catheter,

- the controller and the housing mechanically cooperate such that rotation of the actuator with respect to the housing slides the housing proximally along and over part of the catheter.

In an application, the controller and the housing mechanically cooperate such that rotation of the actuator in a first direction with respect to the housing slides the housing proximally with respect to the actuator, and rotation of the actuator in a second, opposite direction with respect to the housing slides the housing distally with respect to the actuator.

In an application, the track is a first track, and the housing further includes a second track that follows a generally-linear path parallel to the longitudinal axis.

In an application, the track is a channel, and the engaging element is a spur that engages the track by protruding into the channel.

In an application, the track is a rail, and the engaging element is a notch that engages the track by receiving the rail.

In an application:

- a first portion of the generally-helical path has a first pitch, a second portion of the generally-helical path has a second pitch, the second portion being distal to the first portion, and the second pitch being greater than the first pitch, and

- the track follows the generally-helical path that has the first portion that has the first pitch and the second portion that has the second pitch.

In an application:



3

the generally-helical path has a pitch that is progressively greater at progressively distal portions of the generally-helical path, and

the track follows the generally-helical path that has the pitch that is progressively greater at progressively distal portions of the generally-helical path.

In an application, the apparatus further includes the implant.

In an application, the apparatus further includes a shaft to which the implant is fixable, the shaft being slidably coupled to the housing, and extending proximally from the housing.

In an application:

the track is a first track,

the engaging element is a first engaging element,

the housing further includes a second track that follows a generally-linear path parallel to the longitudinal axis,

the tool further includes a second engaging element, fixedly coupled to the shaft, the second engaging element engaging the second track such that the shaft is rotationally fixed with respect to the housing.

In an application, the controller and the housing mechanically cooperate such that rotation of the actuator with respect to the housing slides the second track longitudinally with respect to the second engaging element.

In an application, the apparatus further includes the implant, fixedly coupled to the shaft, at least the part of the implant housed by the housing.

In an application, the rod is coaxial with the shaft.

In an application, the shaft is disposed within the rod.

In an application, the actuator defines a hole through which the shaft extends.

In an application, the shaft is rotationally fixed with respect to the housing.

In an application, at least part of the shaft is disposed within the housing.

There is further provided, in accordance with an application of the present invention, a method, including:

transluminally advancing, into a heart of a subject, a distal part of a tool, the distal part of the tool including a housing, the housing:

including a tubular wall that circumscribes a longitudinal axis of the distal part of the tool,

housing at least part of an implant, and

defining a track that follows a generally-helical path around the longitudinal axis; and

retracting the housing from at least the part of the implant by rotating a rod that is fixedly coupled to an actuator that includes an engaging element that is engaged with the track, such that the actuator rotates with respect to the housing and causes the housing to slide longitudinally with respect to the actuator.

There is further provided, in accordance with an application of the present invention, apparatus, including:

an implant; and

a tool, configured for transluminal delivery of the implant, the tool having a proximal part and a distal part, and including:

a shaft that extends longitudinally from the proximal part of the tool to the distal part of the tool;

a nosepiece, fixed to the shaft, and arranged with respect to the implant such that the implant extends proximally away from the nosepiece and over the shaft;

a sheath, configured to house the implant during transluminal delivery, and having a diameter that is dimensioned for transluminal delivery; and

4

a balloon, disposed at the distal part of the tool, and in fluid communication with the proximal part of the tool,

and the balloon has:

a maximally-inflated state in which the balloon (i) has a widest part that has an inflated diameter that is less than the diameter of the sheath or at most 10 percent greater than the diameter of the sheath, and (ii) has a tapered portion that tapers longitudinally away from the widest part and from the nosepiece, and

a deflated state in which the widest part has a deflated diameter that is smaller than the inflated diameter.

In an application, the nosepiece is fixed to the distal end of the shaft.

In an application, the tapered portion tapers distally away from the widest part and from the nosepiece.

In an application, the tapered portion tapers proximally away from the widest part and from the nosepiece.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and

the balloon is in its maximally-inflated state.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and

the balloon is in its deflated state.

In an application, the balloon is slidably coupled to the shaft at least in the deflated state of the balloon.

In an application:

the implant (i) is constrainable, by a constraining force, in a compressed state in which the implant has a compressed diameter, and (ii) has an expanded state into which the implant automatically transitions upon removal of the constraining force, and in which the implant has an expanded diameter, and

the maximally-inflated diameter of the balloon is smaller than the expanded diameter of the implant.

In an application:

the implant is shaped to define a lumen therethrough,

the nosepiece is arranged with respect to the implant such that the implant extends proximally over the shaft with the shaft within the lumen of the implant,

the implant has an expanded state, and assumes the expanded state upon implantation of the implant, and the nosepiece is dimensioned to be withdrawable proximally through the lumen while the implant is in its expanded state.

In an application, the implant is self-expanding to the expanded state.

In an application, the implant has a compressed state for transluminal delivery, and the nosepiece is not dimensioned to be withdrawable proximally through the lumen while the implant is in its compressed state.

There is further provided, in accordance with an application of the present invention, apparatus, including:

an implant:

constrainable, by a constraining force, in a compressed state in which the implant has a compressed diameter,

having an expanded state into which the implant automatically transitions upon removal of the constraining force, and in which the implant has an expanded diameter; and



## 5

a tool, configured for transluminal delivery of the implant, the tool including:  
 a shaft that extends longitudinally from a proximal part of the tool;  
 a nosepiece, fixed to the shaft, and arranged with respect to the implant such that the implant extends proximally away from the nosepiece and over the shaft; and  
 a balloon, in fluid communication with the proximal part of the tool, and the balloon has:  
 a maximally-inflated state in which the balloon (i) has a widest part that has an inflated diameter that is smaller than the expanded diameter, and (ii) has a tapered portion that tapers longitudinally away from the widest part and from the nosepiece, and  
 a deflated state in which the widest part has a deflated diameter that is smaller than the inflated diameter.

In an application, the nosepiece is fixed to the distal end of the shaft.

In an application, the tapered portion tapers distally away from the widest part and from the nosepiece.

In an application, the tapered portion tapers proximally away from the widest part and from the nosepiece.

In an application, the balloon is slidably coupled to the shaft at least in the deflated state of the balloon.

In an application:

the implant (i) is constrainable, by a constraining force, in a compressed state in which the implant has a compressed diameter, and (ii) has an expanded state into which the implant automatically transitions upon removal of the constraining force, and in which the implant has an expanded diameter, and

the maximally-inflated diameter of the balloon is smaller than the expanded diameter of the implant.

In an application:

the implant is shaped to define a lumen therethrough, the nosepiece is arranged with respect to the implant such that the implant extends proximally over the shaft with the shaft within the lumen of the implant,

the implant has an expanded state, and assumes the expanded state upon implantation of the implant, and the nosepiece is dimensioned to be withdrawable proximally through the lumen while the implant is in its expanded state.

In an application, the implant is self-expanding to the expanded state.

In an application, the implant has a compressed state for transluminal delivery, and the nosepiece is not dimensioned to be withdrawable proximally through the lumen while the implant is in its compressed state.

In an application, the tool further includes a sheath that is configured to house the implant during transluminal delivery, and has a diameter that is dimensioned for transluminal delivery.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and  
 the balloon is in its maximally-inflated state.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and  
 the balloon is in its deflated state.

## 6

There is further provided, in accordance with an application of the present invention, apparatus, including:

an implant; and

a tool, configured for transluminal delivery of the implant, the tool including:

a shaft that extends longitudinally from a proximal part of the;

a nosepiece, fixed to the shaft, and arranged with respect to the implant such that the implant extends proximally away from the nosepiece and over the shaft; and

a balloon, inflatable from a proximal part of the tool, and coupled to the shaft such that when inflated the balloon has a tapered portion that tapers distally away from the nosepiece.

In an application, the nosepiece is fixed to the distal end of the shaft.

In an application:

the implant:

is constrainable, by a constraining force, in a compressed state in which the implant has a compressed diameter, and

has an expanded state into which the implant automatically transitions upon removal of the constraining force, and in which the implant has an expanded diameter; and

the balloon has:

a maximally-inflated state in which (i) the balloon has a widest part that has an inflated diameter that is smaller than the expanded diameter of the implant, and (ii) the tapered portion tapers distally away from the nosepiece and from the widest part, and

a deflated state in which the widest part has a deflated diameter that is smaller than the inflated diameter.

In an application, the balloon is slidably coupled to the shaft at least in the deflated state of the balloon.

In an application:

the implant is shaped to define a lumen therethrough, the nosepiece is arranged with respect to the implant such that the implant extends proximally over the shaft with the shaft within the lumen of the implant,

the implant has an expanded state, and assumes the expanded state upon implantation of the implant, and the nosepiece is dimensioned to be withdrawable proximally through the lumen while the implant is in its expanded state.

In an application, the implant is self-expanding to the expanded state.

In an application, the implant has a compressed state for transluminal delivery, and the nosepiece is not dimensioned to be withdrawable proximally through the lumen while the implant is in its compressed state.

In an application, the tool further includes a sheath that is configured to house the implant during transluminal delivery, and has a diameter that is dimensioned for transluminal delivery.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and  
 the balloon is in its maximally-inflated state.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and



the balloon is in its deflated state.

There is further provided, in accordance with an application of the present invention, apparatus, including:

an implant; and

a tool, configured for transluminal delivery of the implant, the tool including:

a shaft that extends longitudinally from a proximal part of the tool to a distal end of the shaft, and has an opening at the distal end, the opening having an opening diameter, and the implant being reversibly coupled to the tool and disposed around the shaft; and

a nosecone:

coupled to the shaft such that the nosecone has (i) a widest part that is disposed outside the opening, and has a diameter that is greater than the opening diameter, and (ii) a tapered portion that tapers distally away from the opening and the implant, and

withdrawable through the opening into the shaft.

In an application, the nosecone is inflatable.

In an application, the tool further includes a sheath that is configured to house the implant during transluminal delivery, and has a diameter that is dimensioned for transluminal delivery.

There is further provided, in accordance with an application of the present invention, apparatus for use with an implant, the apparatus including a delivery tool, the delivery tool including:

a sheath that defines a cavity dimensioned to house at least a portion of the implant, and has a lip that defines a proximal opening via which the portion of the implant is removable from the cavity;

a shaft that:

extends longitudinally from a proximal part of the tool to the sheath, and

is coupled to the sheath such that shaft passes through the proximal opening, and the lip circumscribes a longitudinal site of the shaft; and

a balloon disposed over the shaft at at least the longitudinal site, and inflation of the balloon obstructs the opening.

In an application, the balloon is positioned and dimensioned such that inflation of the balloon brings the balloon in contact with the lip.

In an application, the sheath has a diameter, and the balloon has a maximally-inflated state in which the balloon has a widest part that has an inflated diameter that is less than the diameter of the sheath or at most 10 percent greater than the diameter of the sheath.

In an application, the balloon has a maximally-inflated state in which the balloon has a tapered portion that tapers proximally away from the opening.

In an application:

the implant (i) is constrainable, by a constraining force, in a compressed state in which the implant has a compressed diameter, and (ii) has an expanded state into which the implant automatically transitions upon removal of the constraining force, and in which the implant has an expanded diameter, and

the balloon has a maximally-inflated state in which the balloon is smaller than the expanded diameter of the implant.

In an application, the balloon has a deflated state for delivery of the implant, and a maximally-inflated state, and inflation of the balloon to the maximally-inflated state obstructs at least 80 percent of the opening.

In an application, when the balloon is in the deflated state, the opening is at least 50 percent unobstructed by either the balloon or the shaft.

In an application, the apparatus has a delivery state in which the implant, the sheath, and the balloon are transluminally advanceable into a subject, and in which:

the implant is in a compressed state, and is housed by the sheath, and

the balloon is in its deflated state.

In an application, in the delivery state the implant is compressed around the balloon.

There is further provided, in accordance with an application of the present invention, apparatus, including:

an implant; and

a tool, configured for transluminal delivery of the implant, the tool including:

a shaft that extends longitudinally from a proximal part of the tool, and has an open distal end, the implant being reversibly coupled to the tool and disposed around a distal portion of the shaft;

a sheath that houses the implant, and has a diameter that is dimensioned for transluminal delivery; and

a control element, disposed within the shaft, movement of the control element within the shaft being controllable by the proximal part of the tool, and the control element being coupled to the sheath such that movement of the control element proximally within the shaft draws the sheath (i) distally off of the implant, and (ii) into the open distal end of the shaft.

In an application, the sheath includes a flexible sheet.

In an application, the sheet is doubled-over itself to define an inner wall of the sheath, and an outer wall of the sheath.

In an application, the sheet defines a proximal opening of the sheath at a transition zone between the inner wall and the outer wall, and the movement of the control element proximally within the shaft peels the sheath distally off of the implant by drawing the outer wall progressively into the open distal end of the shaft such that progressively proximal regions of the inner wall transition through the transition zone to become part of the outer wall, and the proximal opening of the sheath moves distally along the implant.

In an application:

the control element includes a shank that extends through the shaft, and a coupling rotatably coupled to a distal end of the shank;

the control element is coupled to the sheath by the coupling being coupled to the sheath; and

the shaft defines an inner screw thread that is complementary to the outer screw thread; and

the control element and the shaft are configured such that rotation of the shank with respect to the sheath provides the movement of the control element proximally within the shaft by (i) screwing the shank through the shaft, but (ii) slides the coupling linearly through the shaft.

In an application, the shaft defines an inner linear groove that extends longitudinally along the shaft, and the coupling defines a fin that extends outward and into the inner groove, disposition of the fin within the groove inhibiting rotation of the coupling with respect to the shaft but allowing longitudinal sliding of the coupling through the shaft.

In an application, the inner screw thread and the inner linear groove are defined by the same longitudinal region of the shaft.

In an application, the inner screw thread and the inner linear groove transect each other.



There is further provided, in accordance with an application of the present invention, a method, for use with a subject, the method including:

transluminally advancing, into a subject, an implant housed within a cavity defined by a sheath of a tool, the tool including a balloon;  
subsequently, intracorporeally removing the implant from the cavity via a proximal opening of the cavity;  
subsequently, obstructing the proximal opening by inflating the balloon; and  
subsequently, while the balloon is inflated, withdrawing the balloon and the sheath via a lumen of the implant.

The present invention will be more fully understood from the following detailed description of applications thereof, taken together with the drawings, in which:

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A-F are schematic illustrations of a system comprising an implant and a tool configured for transluminal delivery of the implant, in accordance with some applications of the invention;

FIGS. 2A-F and 3 are schematic illustrations of another system comprising the implant and a tool configured for transluminal delivery of the implant, in accordance with some applications of the invention; and

FIGS. 4A-D are schematic illustrations of another system comprising the implant and a tool configured for transluminal delivery of the implant, in accordance with some applications of the invention;

FIG. 5 is a schematic illustration of another system comprising the implant and a tool configured for transluminal delivery of the implant, in accordance with some applications of the invention;

FIGS. 6A-C and 7A-C are schematic illustrations of a tool for use with an implant, in accordance with some applications of the invention; and

FIG. 8 is a schematic illustration of an alternative tool, in accordance with some applications of the invention.

#### DETAILED DESCRIPTION OF EMBODIMENTS

Reference is made to FIGS. 1A-F and to FIGS. 2A-F and 3, which are schematic illustrations of a system 100 and a system 200, respectively, in accordance with some applications of the invention. Each of systems 100 and 200 comprises an implant 20 and a tool 110 (system 100) or 210 (system 200), the tool configured for transluminal delivery of the implant. For some applications, and as shown, implant 20 is a prosthetic heart valve (e.g., a prosthetic mitral valve). However, implant 20 may alternatively be a different type of implant. Typically, implant 20 comprises a tubular portion 22 that defines a lumen 24 through the implant (at least in an implanted and/or expanded state of the implant). Implant 20 may further comprise additional features such as anchoring elements (not shown). For applications in which implant 20 is a prosthetic valve, the implant further comprises a valve member, such as one or more prosthetic leaflets, disposed within lumen 24.

Each of tools 110 and 210 is configured for transluminal delivery of implant 20, and has a proximal part (e.g., a proximal part 112 of tool 110; the proximal part of tool 210 may be similar, mutatis mutandis) and a distal part 114 (tool 110) or 214 (tool 210). The proximal part is typically an extracorporeal part (e.g., comprising a handle, port(s) and/or controllers), and the distal part is transluminally advance-

able into a subject (e.g., to the heart of the subject). Each of tools 110 and 210 further comprises:

- (1) a shaft 116 (tool 110) or 216 (tool 210) that extends longitudinally from the proximal part of the tool to the distal part of the tool;
- (2) a nosepiece 118 (tool 110) or 218 (tool 210), fixed to the shaft (e.g., to the distal end of the shaft), and arranged with respect to the implant such that the implant extends proximally away from the nosepiece and over the shaft (e.g., with the shaft disposed within a lumen defined by the implant); and
- (3) a balloon 120 (tool 110) or 220 (tool 210) disposed at the distal part of the tool, and in fluid communication with the proximal part of the tool (e.g., inflatable from the proximal part of the tool).

Each of balloons 120 and 220 has (i) a maximally-inflated state in which the balloon has a widest part (122 or 222, respectively) that has an inflated diameter (d101 or d201, respectively), and a tapered portion (124 or 224, respectively) that tapers longitudinally away from the widest part and from the nosepiece, and (ii) a deflated state in which the widest part has a deflated diameter that is smaller than the inflated diameter. The maximally-inflated state of balloon 120 is shown, for example, in FIG. 1A, and the maximally-inflated state of balloon 220 is shown, for example, in FIGS. 2E-F.

Balloons 120 and 220 are not configured (e.g., dimensioned or arranged with respect to implant 20) for expanding implant 20 at the implant site. Rather, the tapered portion facilitates smooth intracorporeal movement of the tool. For example, and as described hereinbelow, balloon 120 facilitates movement of tool 110 distally through the vasculature of the subject, and balloon 220 facilitates withdrawal of tool 210 from implant 20.

Typically, each of tools 110 and 210 further comprises a sheath (126 or 226, respectively), configured to house the implant (e.g., at least part of the implant) during transluminal delivery, and having a diameter (d102 or d202, respectively) that is dimensioned for transluminal delivery.

Typically, implant 20 is an expandable implant, having a compressed diameter d1 (FIG. 1A) for transluminal delivery, and an expanded diameter d2 (FIG. 1E) for functioning at the implant site. Typically, the compressed and expanded diameters refer to those of tubular portion 22 (rather than those of any additional features such as an anchoring element). For example, implant 20 (e.g., tubular portion 22) may be self-expanding (e.g., comprising a shape-memory material such as Nitinol), such that it (i) is constrainable in a compressed state by a constraining force, and (ii) has an expanded state into which it automatically transitions upon removal of the constraining force. For such applications, the constraining force is typically provided by a sheath, such as sheath 126 of tool 110 or housing 426 of tool 410, and removal of the constraining force occurs when the implant becomes deployed from the sheath.

For some applications, the maximally-inflated diameter of the balloon is smaller than expanded diameter d2 of implant 20 (e.g., the expanded diameter of tubular portion 22). For example, the inflated diameter of the balloon may be less than 90 percent (e.g., less than 80 percent, e.g., less than 70 percent, e.g., less than 60 percent, e.g., less than 50 percent, e.g., less than 40 percent, e.g., less than 30 percent, e.g., less than 20 percent, e.g., less than 10 percent) of the expanded diameter of the implant. It is to be noted that balloons 120 and 220 thus differ from balloons used for expanding plastically-expandable implants, inter alia, in this regard because such implant-expanding balloons necessarily



## 11

expand to a diameter that is significantly greater than that of the compressed diameter of the implant, in order to expand the implant from its delivery state to its expanded state at the implantation site.

For some applications, the inflated diameter of the balloon is less than the diameter of the sheath or is at most 10 percent greater than the diameter of the sheath. For example, the inflated diameter of the balloon may be 20-110 percent, (such as 20-100 percent, or 30-110 percent) the diameter of the sheath, e.g., 30-110 percent (such as 30-100 percent or 40-110 percent), e.g., 40-110 percent (such as 40-100 percent or 50-110 percent), e.g., 50-110 percent (such as 50-100 percent or 60-110 percent), e.g., 60-110 percent (such as 60-100 percent or 70-110 percent), e.g., 70-110 percent (such as 70-100 percent or 80-110 percent), e.g., 80-110 percent (such as 80-100 percent or 90-110 percent), e.g., 90-110 percent (such as 90-100 percent or 100-110 percent). The inflated diameter of the balloon may be less than 90 percent (e.g., less than 80 percent, e.g., less than 70 percent, e.g., less than 60 percent, e.g., less than 50 percent) the diameter of the sheath. It is to be noted that balloons **120** and **220** thus differ from balloons used for expanding plastically-expandable implants, inter alia, in this regard because such implant-expanding balloons necessarily expand to a diameter that is significantly greater than that of the sheath, in order to expand the implant from its delivery state within the sheath, to its expanded state at the implantation site.

Reference is now made to FIGS. 1A-F. System **100** comprises implant **20**, and tool **110**. Tool **110** is configured for transluminal delivery of the implant, and comprises shaft **116**, nosepiece **118**, and balloon **120**. In its maximally-inflated state (FIG. 1A), tapered portion **124** of balloon **120** tapers distally away from nosepiece **118** (and typically from implant **20**). Balloon **120** (or tapered portion **124** thereof) therefore defines a nosecone **128** of tool **110**, the nosecone facilitating transluminal advancement of the tool, such as transfemoral advancement into the aorta and/or transseptal advancement into the left atrium **6**.

It is to be noted that the term “maximally-inflated state” (including in the specification and the claims) means the state in which the balloon has the inherent maximum volume provided by the dimensions into which the material from which it is made is formed (e.g., the maximum inflation before plastic deformation and/or rupture occurs).

FIG. 1A thus shows system **100** in a delivery state thereof, in which the implant, the sheath, and the balloon are transluminally advanceable into a subject. In the delivery state of system **100**, (i) implant **20** is in a compressed state, and is housed by the sheath **126**, and (ii) balloon **120** is in its maximally-inflated state. For some applications, diameter **101** of balloon **120** in its maximally-inflated state is 1-9 mm (e.g., 3-6 mm).

Nosecones are known in the art for advancement of devices (e.g., tools, catheters, etc.) through the vasculature. However, the presence of such nosecones adds to the length of the device. For some applications, it is important to reduce the length of the device, or particular parts thereof. For example, a delivery tool for transseptal (e.g., transfemoral) implantation of a prosthetic mitral valve (e.g., tool **110**) turns sharply downward after passing through the interatrial septum **7** (e.g., at the fossa ovalis) in order (i) to pass between the leaflets of the native mitral valve **10**, and (ii) to be angled (or to angle the implant therewithin) appropriately for implantation (e.g., perpendicular to the native mitral valve). The required sharpness of this turn is at least partly dictated by (i) the height **d4** of atrium **6** from mitral valve **10** (e.g., the mitral annulus) to the ceiling of the atrium, (ii) the

## 12

height **d5** between the mitral valve and the entry point **5** of tool **110** through septum **7** (e.g., the fossa ovalis), and/or (iii) the distance across atrium **6**, perpendicular to heights **d4** and **d5**, between septum **7** and the target site—typically the center of mitral valve **10**.

Because nosecone **128** is defined by balloon **120**, the length of tool **110** (e.g., distal part **114** thereof) is reducible by at least deflating balloon **120**. Deflation is typically performed after passage through septum **7** and before the turning of distal part **114** toward native mitral valve **10**, thereby facilitating this turning.

Typically, when in its deflated state, balloon **120** is withdrawable into an opening **130** at the distal end of shaft **116**, whereas inflated diameter **d101** is greater than the diameter of opening **130**. Therefore, nosecone **128** defined by balloon **120** is:

(1) coupled to shaft **116** such that the nosecone has (i) a widest part **122** that is disposed outside opening **130**, and has a diameter **d101** that is greater than the opening diameter, and (ii) a tapered portion **124** that tapers distally away from the opening and implant **20**, and

(2) withdrawable (e.g., slidable) through opening **130** into shaft **116**.

Balloon **120** is typically fixed to a control rod **134** that is slidable within shaft **116**. Control rod **134** is typically slidable over a guidewire **136** (e.g., the rod has a first lumen **138** within which the guidewire is disposed). Balloon **120** is typically also inflatable and deflatable via control rod **134**, which may have a secondary lumen **140** (e.g., parallel with or coaxially surrounding the lumen **138**) that has one or more openings **132** into balloon **120**. Therefore, at least in its deflated state, balloon **120** is slidably coupled to shaft **116** (e.g., via rod **134**).

FIG. 1B shows balloon **120** in its deflated state, and FIG. 1C shows the balloon having been subsequently withdrawn into shaft **116**, thereby reducing the overall length of tool **110**. Subsequently, distal part **114** of tool **110** is steered toward native mitral valve **10**, and between the leaflets thereof (FIG. 1D). As described hereinabove, the prior reduction in the length of tool **110** reduces a likelihood of tissue of the heart interfering with this steering. Typically, this steering is achieved using a steerable mid-portion **113** (e.g., a steerable catheter) that extends from proximal part **112** to distal part **114**, and through which shaft **116** extends.

Once distal part **114** of the tool **110** is positioned at the implantation site (e.g., at native mitral valve **10**), implant **20** is deployed from sheath **126**. FIG. 1E shows implant **20** having expanded, upon deployment, into its expanded state. Typically, implant **20** is a self-expanding implant, e.g., comprising Nitinol or another elastic material. Typically, despite this expansion, shaft **116** remains disposed through a lumen defined by the implant until it, and nosepiece **118**, are withdrawn proximally through the lumen (FIG. 1F). For some applications, nosepiece **118** is not dimensioned to be withdrawable proximally through the lumen of implant **20** while the implant is in its compressed state. For example, implant **20** may be fixed to nosepiece **118** while in its compressed state, such that the nosepiece serves as an implant controller. For example, while nosepiece **118** is in one position with respect to sheath **126** it may maintain implant **20** within the sheath, and deployment of the implant may be executed by relative movement between the nosepiece and the sheath (e.g., controlled from the proximal part of tool **110**).

Sheath **126** is not shown in FIGS. 1E-F, reflecting that, for some embodiments, sheath **126** is a flexible sheath that is drawn into shaft **116** during deployment of implant **20** (e.g.,



as described for sheath 326 with reference to FIGS. 4A-D, *mutatis mutandis*). However, it is to be noted that for some applications, sheath 126 is rigid (e.g., is a capsule) and is withdrawn while remaining disposed over part of shaft 116. (For such applications, sheath 126 would be visible in FIGS. 1E-F.)

There is therefore provided, a method, comprising: (1) transluminally advancing, into a subject, an implant housed within a cavity defined by a sheath of a tool, the tool including a balloon; (2) subsequently, intracorporeally removing the implant from the cavity via a proximal opening of the cavity; (3) subsequently, obstructing the proximal opening by inflating the balloon; and (4) subsequently, while the balloon is inflated, withdrawing the balloon and the sheath via a lumen of the implant.

Reference is now made to FIGS. 2A-F, and 3. System 200 comprises implant 20, and tool 210. Tool 210 is configured for transluminal delivery of the implant, and comprises shaft 216, nosepiece 218, and balloon 220. As described in more detail hereinbelow, in its maximally-inflated state (FIGS. 2E-F), tapered portion 224 of balloon 220 tapers proximally away from nosepiece 218.

FIG. 2A shows system 200 in a delivery state thereof, in which implant 20, sheath 226, and balloon 220 are transluminally advanceable into a subject, toward a delivery site (e.g., mitral valve 10). In the delivery state of system 200, (i) implant 20 is in a compressed state, and is housed by the sheath 226 (which typically constrains the implant in the compressed state), and (ii) balloon 220 is in its deflated state.

Sheath 226 defines a cavity 242 that is dimensioned to house at least a portion of implant 20, and has a lip 232 that defines a proximal opening 230 via which the housed portion of the implant is removable from the cavity. For some applications, sheath 226 comprises a distal piece 226*d* and a proximal piece 226*p* that face each other and house respective portions of implant 20, and the distal piece defines cavity 242 and proximal opening 230. (Sheath 226 may alternatively comprise only one piece, shaped generally like distal piece 226*d*.)

Shaft 216 extends longitudinally from the proximal part of the tool to distal part 214, at which sheath 226 and nosepiece 218 are disposed. Shaft 216 is coupled to the sheath such that shaft passes through proximal opening 230, and lip 232 circumscribes a longitudinal site 235 of the shaft. Typically, balloon 220 is disposed over the shaft at at least longitudinal site 235.

Shaft 216 extends through the lumen defined by implant 20, and is fixed to nosepiece 218, which is disposed distally to the implant. Typically, nosepiece 218 is fixed to sheath 226 (e.g., distal piece 226*d* thereof). For some applications, and as shown, sheath 226 (e.g., distal piece 226*d* thereof) is fixed to shaft 216 via nosepiece 218 (i.e., by being connected to the nosepiece, which itself is connected to the sheath). Typically, nosepiece 218 is fixed to the distal end of shaft 216. Nosepiece 218 serves as a nosecone 219; the advantages of a nosecone are described hereinabove. Typically, nosepiece 218 is not dimensioned to be withdrawable proximally through the lumen of implant 20 while the implant is in its compressed state.

Tool 210 is typically advanced to the implantation site over a guidewire 236. For example, shaft 216, sheath 226, and/or nosepiece 218 are shaped to define a lumen 244 through which guidewire 236 is slidable.

Once at the implantation site, the housed portion of implant 20 is removed from cavity 242 by moving distal piece 226*d* distally with respect to the implant (FIG. 2B). In addition, proximal piece 226*p* may be moved proximally

with respect to the implant. Implant 20 is deployed by sufficiently (e.g., fully) exposing it from sheath 226. For applications in which implant 20 is self-expanding, the implant expands automatically after the constraining force provided by sheath 226 has been removed by sufficiently exposing the implant from the sheath.

FIG. 2C shows system 200 after implant 20 has been deployed from sheath 226. Nosepiece 218, distal piece 226*d* of sheath 226, and at least most (e.g., all) of balloon 220 are disposed distally to implant 20. For delivery tools that house an implant in a sheath that has a proximal opening (e.g., a two-piece sheath such as sheath 226, or a sheath that has only one piece shaped generally like distal piece 226*d*), withdrawal of the sheath after implantation of the implant is typically performed by withdrawing the sheath through the lumen of the implant. For example, in the case of a prosthetic valve, the sheath is typically withdrawn through the prosthetic valve, passing between its prosthetic leaflets. A risk exists that, should the distal part of the implantation tool be imperfectly aligned with the implanted implant, the lip (that defines the proximal opening through which the implant was previously withdrawn) may engage (e.g., catch onto) the implant, making withdrawal difficult and/or dislodging the implant. Balloon 220 reduces this risk.

Either before (as shown) or after implantation of implant 20, guidewire 236 is removed from lumen 244. For some applications, lumen 244 is in fluid communication with balloon 220, and the balloon is inflated via this lumen. For some such applications, this fluid communication is provided by a port 246 defined by shaft 216, and balloon 220 is inflated by delivering a fluid 238 (e.g., saline) via shaft 216, e.g., via the lumen 244 in which guidewire 236 was previously disposed. Because lumen 244 is open at a distal end, in order to provide fluid pressure for inflating balloon 220, a control rod 248 that is slidable within shaft 216 is slid into lumen 244 prior to inflation. Control rod 248 comprises a distal plug 250 that fits snugly within at least a distal region 244*d* of lumen 244 (distal to port 246), such that when the plug is introduced, it seals against the walls of lumen 244 (or at least distal region 244*d* thereof). For example, plug 250 may have an outer diameter that is at least 50 (e.g., at least 70, e.g., at least 90, such as at least 95) percent of the inner diameter of lumen 244. For some applications, and as shown, distal region 248*d* is defined by nosepiece 218 (e.g., nosecone 219). For some applications, and as shown, plug 250 defines an external screw thread 254, and is screwed into distal region 248*d*. For example, nosepiece 218 may comprise a flexible material such as silicone into which screw thread 254 may cut. (Alternatively, distal region 248*d* may be lined with such a material.) The flexible material may advantageously increase atraumatic properties of nosecone 219.

Control rod 248 further comprises a flexible proximal portion 252, which has a diameter that is less than 90 percent (e.g., 20-60 percent) of the inner diameter of lumen 244. Control rod 248 is dimensioned such that, while distal plug 250 is disposed at distal region 248*d* of lumen 244, proximal portion 252 extends distally through lumen 244 at least until port 246. Fluid introduced into lumen 244 at the proximal part of tool 210 flows along the lumen, alongside portion 252, and out of port 246, thereby inflating balloon 220 (FIG. 2E). Plug 250 inhibits the fluid from escaping at distal part 214 of tool 210.

It is to be noted that the scope of the invention includes other techniques for inflating balloon 220. For example, for some applications, shaft 216 may have a secondary lumen



that opens into balloon 220, e.g., as described for lumen 140 of control rod 134 of system 100, mutatis mutandis.

FIG. 2E shows balloon 220 in its maximally-inflated state. Inflation of balloon 220 obstructs opening 230. For some applications, and as shown, inflation of balloon 220 obstructs at least 80 percent (e.g., at least 90 percent) of opening 230, e.g., obstructs opening 230 completely (e.g., sealing up the opening). For example, widest part 222 may have an inflated diameter that is equal to, or slightly (e.g., 1-10 percent) greater than the diameter of opening 230, and balloon 220 comes into contact with (e.g., seals against) lip 232 when inflated. For some applications, inflation of the balloon obstructs 80-90 percent or 90-99 percent of opening 230. In contrast, in the deflated state of balloon 220, opening 230 is typically at least 50 percent (e.g., 60-90 percent) unobstructed by the balloon and/or shaft 216. The obstruction of opening 230 caused by inflation of balloon 220 reduces the risk of lip 232 engaging implant 20 during withdrawal. Because this functionality is provided by a balloon, when the balloon is deflated, cavity 242 is available to house at least part of implant 20.

FIG. 2F shows distal part 214 of tool 210 being withdrawn via the lumen of implant 20, while balloon 220 (e.g., tapered portion 224 thereof) slides past parts of the implant that lip 232 may otherwise have engaged. FIG. 3 illustrates what may occur during withdrawal if balloon 220 is not inflated (or what may occur in a similar system that does not comprise balloon 220), and therefore demonstrates an advantage of system 200. In FIG. 3, lip 232 engages part of implant 20 (e.g., part of the implant enters cavity 242 via opening 230), impeding withdrawal of distal piece 226d and/or causing dislodgement of implant 20.

Reference is made to FIGS. 4A-D, which are schematic illustrations of a system 300, which comprises implant 20, and a tool 310 configured for transluminal delivery of the implant. Tool 310 comprises a shaft 316 that extends longitudinally from a proximal part 312 of the tool (which typically comprises a handle and/or controller), and has an open distal end 330. Implant 20 is reversibly coupled to the tool, and is disposed around a distal portion of shaft 316. Tool 310 comprises a sheath 326 that houses implant 20, and has a diameter that is dimensioned for transluminal delivery. Tool 310 further comprises a control element 334, disposed within shaft 316. Movement of control element 334 within shaft 316 is controllable by proximal part 312 of tool 310, and control element 334 is coupled to sheath 326 such that movement of the control element proximally within the shaft draws the sheath (i) distally off of implant 20, and (ii) into open distal end 330 of the shaft.

Typically, sheath 326 comprises a flexible sheet 328, such as a sheet or fabric of a polymer (e.g., nylon, polytetrafluoroethylene, polyester, or polyethylene terephthalate).

For some applications, sheet 328 defines sheath 326 as a single-walled sheath, and as it is drawn distally off of implant 20, it slides directly over implant 20 (e.g., is in contact with the implant).

For some applications, and as shown, sheet 328 is doubled-over itself to define an inner wall 329a of sheath 326 (i.e., defines the sheath as a double-walled sheath), and an outer wall 329b of the sheath (FIG. 4A). For such applications, a proximal opening 332 of sheath 326 is defined at a transition zone 336 between inner wall 329a and outer wall 329b (i.e., the zone at which sheet 328 transitions between defining the inner wall and defining the outer wall). That is, the transition zone defines a lip of the sheath, the lip defining proximal opening 332. The above-described movement of control element 334 proximally within shaft 316

draws (e.g., peels) sheath 326 distally off of implant 20 by drawing outer wall 329b progressively into open distal end 330 of the shaft such that progressively proximal regions of inner wall 329a transition through transition zone 336 to become part of the outer wall, and the transition zone (and thereby proximal opening 332 of the sheath) moves distally along the implant, exposing progressively distal regions of the implant (FIGS. 4B-C).

Inner wall 329a is typically in contact with implant 20 (e.g., constraining the implant to its compressed diameter), but outer wall 329b is not in contact with the implant. During the unsheathing of implant 20, neither inner wall 329a nor outer wall 329b slides directly over the implant while in contact with the implant. Rather, outer wall 329b slides over inner wall 329a (e.g., while in contact with the inner wall), and the sheath effectively peels off of the implant, thereby advantageously reducing friction that might be caused by direct sliding of the sheath over the implant while in contact with the implant.

FIG. 4D shows sheath 326 having been completely drawn off of implant 20, and the implant having responsively expanded.

Reference is now made to FIG. 5, which is a schematic illustration of a system 300a, which is an embodiment of system 300, in accordance with some applications of the invention. Elements in FIG. 5 that have a reference numeral suffixed "a" are equivalent, mutatis mutandis, to elements in FIGS. 4A-D that have the same reference numeral (without the suffix), except where noted. FIG. 5 shows the state of system 300a that is equivalent to the state of system 300 shown in FIG. 4B, mutatis mutandis.

As described for system 300, movement of control element 334a within shaft 316a is controllable by a proximal part of tool 310a, and control element 334a is coupled to sheath 326a such that movement of the control element proximally within the shaft draws the sheath (i) distally off of implant 20, and (ii) into open distal end 330a of the shaft. In system 300a, this movement of control element 334a is achieved by rotating the control element within shaft 316a. Shaft 316a and control element 334a define, respectively, complementary inner screw thread 342 and outer screw thread 344. FIG. 5 includes an enlarged inset view that shows shaft 316a as though it were opened up flat. Control element 334a comprises a shank 345, and a coupling 346, typically at a distal end of the control element, that is rotatably coupled to shank 345 (e.g., via a bearing 348). Coupling 346 is the portion of control element 334a that is coupled to sheath 326a. Due to mating of threads 342 and 344, rotation of shank 345 within shaft 316a causes control element 334a as a whole to move proximally within the shaft, while coupling 346 remains relatively rotationally stationary with respect to the shaft (e.g., coupling 346 slides longitudinally without rotating), thereby causing sheath 326a to be drawn (i) distally off of implant 20, and (ii) into open distal end 330a of the shaft, without the rotation of shank 345 twisting the sheath. That is, rotation of shank 345 within shaft 316a causes (i) screwing of the shank through the shaft, but (ii) sliding (e.g., linear sliding) of coupling 346 through the shaft.

For some applications, coupling 346 rotates slightly with respect to shaft 316a, but remains relatively rotationally stationary with respect to the shaft due to resistance provided by sheath 326a. For some applications, coupling 346 defines one or more fins 350 that each protrudes radially outward, and into a respective longitudinal groove 352 defined by shaft 316a. Fins 350 can slide only linearly along grooves 352, thereby inhibiting rotation of coupling 346



with respect to shaft **316a**, but allowing the coupling to slide longitudinally along the shaft. For some applications, and as shown, grooves **352** and thread **342** may be defined on the same longitudinal region of shaft **316a**, and may in fact transect each other.

Reference is made to FIGS. **6A-C** and **7A-C**, which are schematic illustrations of a tool **410**, for use with an implant such as implant **20**, in accordance with some applications of the invention. Typically, tool **410** is a delivery tool for transluminal delivery of implant **20**. A system **400** may be provided, comprising implant **20** and tool **410**.

Tool **410** comprises a housing (e.g., a sheath) **426** at a distal part **414** of the tool. Housing **426** comprises a tubular wall **428** that circumscribes a longitudinal axis **ax1** of the distal part of tool **410**. Housing **426** is dimensioned to house at least part of implant **20**. Housing **426** (e.g., wall **428** thereof) defines a track **430** that follows a generally-helical path around longitudinal axis **ax1**. Tool **410** further comprises a controller **440** that comprises a rod **442** and an actuator **444**. Rod **442** extends from a proximal part of the tool to housing **426**. Actuator **444** is rotatable with respect to housing **426**, and is typically fixedly coupled to rod **442**. Actuator **444** comprises an engaging element **446** that engages track **430**. Controller **440** and housing **426** mechanically cooperate such that rotation of actuator **444** with respect to the housing (e.g., by rotation of rod **442**) slides the housing longitudinally with respect to the actuator.

Typically, this movement is bidirectional. That is, rotation of actuator **444** in a first direction with respect to housing **426** slides the housing proximally with respect to the actuator, and rotation of the actuator in a second, opposite direction with respect to the housing slides the housing distally with respect to the actuator.

Typically, and as shown, housing **426** is dimensioned to house implant **20** such that track **430** is disposed around at least the part of implant **20**. That is, typically, at least part of implant **20** is coincident, along axis **ax1**, with at least part of track **430**.

For some applications, housing **426** defines more than one track **430**, rotationally-offset from each other e.g., in order to evenly distribute forces applied by actuator **444** (which for such applications typically comprises a corresponding more than one engaging element **446**). For example, and as shown, housing **426** may define two tracks **430a** and **430b**, rotationally-offset by 180 degrees from each other, and actuator **444** may comprise a corresponding two engaging elements **446**, also rotationally-offset by 180 degrees from each other. For the sake of clarity, reference numerals **430a** and **430b** are only used in FIG. **6A**.

Typically, tool **410** further comprises a catheter **413** (e.g., a mid-portion of the tool), longitudinally disposed between the proximal part of the tool, such as a control handle, and distal part **414**. Housing **426** is typically disposed distally to catheter **413**. Rod **442** extends through catheter **413**, and typically into housing **426**. The mechanical cooperation between controller **440** and housing **426** is such that, to retract the housing from implant **20** (i.e., to deploy the part of the implant housed by the housing) rotation of actuator **444** with respect to the housing slides the housing proximally along and over part of the catheter. This is illustrated in FIGS. **7A-C**, which show progressive steps in the retraction of housing **426** to deploy implant **20**. Distances **d6**, **d7**, and **d8** are each measured along catheter **413**, between a given point on the catheter (e.g., a point of entry into atrium **6**) and housing **426**. Distance **d7** is smaller than distance **d6**, and distance **d8** is smaller than distance **d7**.

As described hereinabove, the dimensions of left atrium **6** limit maneuverability when implanting an implant at mitral valve **10** transseptally (e.g., transfemorally). For example, the height **d4** of atrium **6**, and/or the height **d5** between the mitral valve and the entry point **5** of a delivery tool through septum **7** (e.g., the fossa ovalis), limit the distance to which the delivery tool can be raised away from the mitral valve in order to withdraw the housing or sheath of the tool from over the implant in order to deploy the implant. In particular, these heights limit the ability to raise the tool away from the mitral valve without moving and/or angling the tool toward entry point **5**, and thereby tilting the implant with respect to the mitral valve. It is hypothesized by the inventors that tool **410** facilitates deployment of an implant at the mitral valve, and/or deployment without tilting the implant, because the retraction of housing **426** over catheter **413** replaces at least some of the otherwise required withdrawal of the delivery tool as a whole. For some applications, and as shown in FIGS. **7A-C**, once catheter **413** and the implant within are in the correct position (FIG. **7A**) deployment of the implant is possible without further movement of catheter **413** (FIGS. **7B-C**).

Tool **410** typically further comprises a shaft **450** to which implant **20** is fixable, the shaft being slidably coupled housing **426**, and extending proximally from the housing. Shaft **450** thereby serves as a mount for implant **20**, and facilitates movement of other parts of tool **410** (e.g., housing **426**) with respect to the implant.

Typically, tool **410** is configured in a manner that inhibits housing **426** from rotating in response to rotation of actuator **444**, because the differential rotation causes the retraction of the housing. Therefore, tool **410** therefore typically comprises a housing-rotation inhibitor **460**. For some applications, and as shown, housing-rotation inhibitor **460** comprises (i) a second track **462** that follows a generally-linear path parallel to longitudinal axis **ax1**, and (ii) a second engaging element **466**. Engaging element **466** is fixedly coupled to shaft **450** (e.g., via a mount **464**), and engages track **462**, thereby rotationally fixing the shaft with respect to housing **426**, while facilitating longitudinal sliding of the shaft with respect to the housing. Therefore, controller **440** and housing **426** mechanically cooperate such that rotation of actuator **444** with respect to the housing slides the track **462** longitudinally with respect to engaging element **466**.

For some applications, housing **426** defines more than one second track **462**, rotationally-offset from each other, e.g., in order to evenly distribute forces applied to it by, for example, a corresponding more than one engaging element **466**. For example, and as shown, housing **426** may define two tracks **462**, rotationally-offset by 180 degrees from each other, and tool **410** may comprise a corresponding two engaging elements **466**, also rotationally-offset by 180 degrees from each other.

Typically, rod **442** is coaxial with shaft **450**. Further typically, shaft **450** is disposed within rod **442** (which is typically disposed within catheter **413**). Typically, actuator **444** defines a hole therethrough, through which shaft **450** extends. For example, at least part of shaft **450** may be disposed within housing **426**, and the shaft extends distally out of catheter **413**, through the hole in actuator **444**, and into the housing.

The term “generally helical” is used with respect to the path of track **430** because the path may not be a true helix. For example, for some applications, and as shown, the pitch of the generally-helical path of the track differs along its length. For some such applications, a first portion **432p** of the generally-helical path has a first pitch, and a second



portion **432d** of the generally-helical path, which is distal to the first portion, has a second pitch that is greater than the first pitch. For example, the pitch of the generally-helical path may gradually increase, such that it is progressively greater at progressively distal portions of the generally-helical path. It is hypothesized by the inventors that this facilitates (i) application of greater linear force during the initial stage of deployment from housing **426**, while more of implant **20** is disposed in the housing and friction between the implant and housing is greater, and (ii) greater linear movement during later stages of deployment from housing **426**, after some of the implant has already exited the housing, and friction between the implant and housing has been reduced. Alternatively or additionally, the distance of track **430** from longitudinal axis **ax1** may differ along its length. For example, housing **426** may be wider toward its distal opening, and track **430**, defined by the housing, may correspondingly become increasingly further from axis **ax1** toward the distal opening of the housing.

Typically, and as shown, track **432** is a channel (e.g., cut into housing **426**, such as into tubular wall **428** thereof), and engaging element **446** is a spur that engages the track by protruding into the channel. However, alternative tracks and engaging elements may be used. For example, and as shown in FIG. **8**, to which reference is now additionally made, the track may be a rail, and the engaging element may be a notch that engages the track by receiving the rail. FIG. **8** is a schematic illustration of alternative tool **510**, in accordance with some applications of the invention. Except where noted, tool **510** is identical to tool **410**, and its components are identical to identically-named components of tool **410**. FIG. **8** shows a transverse cross-section of tool **510** that substantially corresponds to the transverse cross-section of tool **410** that is shown in FIG. **6C**. As shown, a track **530** (which substantially corresponds to track **430** of tool **410**) is a rail that protrudes radially-inward from a tubular wall **528** of a housing **526**, and an engaging element **546** is a notch defined by an actuator **544**, the notch receiving the rail.

Second track **462** and second engaging element **466** are shown as a channel and spur, but may, alternatively or additionally, be similarly substituted with a rail and notch, *mutatis mutandis*. For example, tool **510** may comprise a shaft **550** to which is fixedly coupled an engaging element (not shown in FIG. **8**), e.g., via a mount **564**.

For some applications, the first track and the first engaging element are of the channel-and-spur type, and the second track and the second engaging element are of the rail-and-notch type. For some applications, the first track and the first engaging element are of the rail-and-notch type, and the second track and the second engaging element are of the channel-and-spur type. For some applications, both are of the channel-and-spur type (e.g., as shown for tool **410**). For some applications, both are of the rail-and-notch type.

Reference is again made to FIGS. **1A-8**. The components of the systems described herein may be combined in various ways. For example, balloon **120** may be used (in addition to or in place of the above-described components) in system **200** and/or in system **300**, *mutatis mutandis*; balloon **220** may be used (in addition to or in place of the above-described components) in system **100** and/or in system **300**, *mutatis mutandis*; and/or sheath **326** may be used (in addition to or in place of the above-described components) in system **100** or in system **200**, *mutatis mutandis*.

Similarly, tool **410**, or elements thereof, may be used in combination with other embodiments described herein. For example, housing **426** may serve as a proximal piece of a sheath (e.g., sheath **226**) that also has a distal piece, housing

**426** being moved proximally to deploy a proximal part of the housed implant, and the distal piece of the sheath being moved distally to deploy a distal part of the housed implant. That is, for some applications, housing **426** is a proximal housing that is dimensioned to house a first part of the implant, and has a distal opening for deployment of the first part of the implant therethrough; and the tool further comprises a distal housing that is dimensioned to house a second part of the implant, and has a proximal opening, facing the distal opening, for deployment of the second part of the implant therethrough. For such applications, both housings are typically independently slidable with respect to the implant, and also with respect to shaft **450**.

The term “diameter,” which is used throughout this application (including the specification and the claims), refers to a dimension of the component that is transverse to the longitudinal axis of the component and/or of the system as a whole. The term “diameter” is used because such components typically have a circular transverse cross-section. However, it is to be understood that the descriptions may equally apply to equivalent components that have a non-circular cross-section, *mutatis mutandis*.

Each of the systems described hereinabove is described as comprising implant **20**. However, it is to be noted that the scope of the invention includes systems that do not comprise an implant—i.e., systems that are otherwise the same as those described, but which are provided as delivery systems for an implant that is not included.

It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described hereinabove. Rather, the scope of the present invention includes both combinations and subcombinations of the various features described hereinabove, as well as variations and modifications thereof that are not in the prior art, which would occur to persons skilled in the art upon reading the foregoing description.

The invention claimed is:

1. Apparatus, comprising:

an implant; and

a tool, configured for transluminal delivery of the implant, the tool comprising:

a shaft that extends longitudinally from a proximal part of the tool, and has an open distal end, the implant being reversibly coupled to the tool and disposed around a distal portion of the shaft;

a sheath that houses the implant, and has a diameter that is dimensioned for transluminal delivery; and

a control element, disposed within the shaft, movement of the control element within the shaft being controllable by the proximal part of the tool, and the control element being coupled to the sheath such that movement of the control element proximally within the shaft draws the sheath (i) distally off of the implant, and (ii) into the open distal end of the shaft,

wherein:

the control element comprises a shank that extends through the shaft, and a coupling rotatably coupled to a distal end of the shank;

the control element is coupled to the sheath by the coupling being coupled to the sheath; and

the shank defines an outer screw thread;

the shaft defines an inner screw thread that is complementary to the outer screw thread; and

the control element and the shaft are configured such that rotation of the shank with respect to the sheath provides the movement of the control element proximally within



## 21

the shaft by (i) screwing the shank through the shaft, but (ii) slides the coupling linearly through the shaft.

2. The apparatus according to claim 1, wherein the sheath comprises a flexible sheet.

3. The apparatus according to claim 2, wherein the sheet is doubled-over itself to define an inner wall of the sheath, and an outer wall of the sheath.

4. The apparatus according to claim 3, wherein the sheet defines a proximal opening of the sheath at a transition zone between the inner wall and the outer wall, and the movement of the control element proximally within the shaft peels the sheath distally off of the implant by drawing the outer wall progressively into the open distal end of the shaft such that progressively proximal regions of the inner wall transition through the transition zone to become part of the outer wall, and the proximal opening of the sheath moves distally along the implant.

5. The apparatus according to claim 1, wherein the shaft defines an inner linear groove that extends longitudinally along the shaft, and the coupling defines a fin that extends outward and into the inner groove, disposition of the fin within the groove inhibiting rotation of the coupling with respect to the shaft but allowing longitudinal sliding of the coupling through the shaft.

6. The apparatus according to claim 5, wherein the inner screw thread and the inner linear groove are defined by the same longitudinal region of the shaft.

7. The apparatus according to claim 5, wherein the inner screw thread and the inner linear groove transect each other.

8. A method, comprising:

transluminally advancing, into a heart of a subject, an implant and a distal part of a tool, the implant being reversibly coupled to the tool, the tool including:

a shaft that extends longitudinally from a proximal part of the tool, and has an open distal end, the implant disposed around a distal portion of the shaft,

a sheath that houses the implant, the sheath having a diameter that is dimensioned for transluminal delivery,

## 22

a control element disposed within the shaft and coupled to the sheath, the control element:

including a shank that extends through the shaft, the shank having an outer screw thread and an inner screw thread that is complementary to the outer screw thread;

having a coupling rotatably coupled to a distal end of the shank;

being coupled to the sheath by the coupling being coupled to the sheath; and

from the proximal part of the tool, drawing the sheath distally off of the implant and into the open distal end of the shaft, by moving the control element proximally within the shaft, by rotating the shank with respect to the sheath such that:

the shank screws through the shaft; and

the coupling slides linearly through the shaft.

9. The method according to claim 8, wherein rotating the shank with respect to the sheath such that the coupling slides linearly through the shaft comprises sliding a fin of the coupling along a longitudinal inner groove of the shaft, such that the fin inhibits rotation of the coupling with respect to the shaft.

10. The method according to claim 8, wherein:

a sheet is doubled-over itself to define an inner wall of the sheath, and an outer wall of the sheath,

the sheet defines a proximal opening of the sheath at a transition zone between the inner wall and the outer wall, and

drawing involves peeling the sheath distally off of the implant by drawing the outer wall of the sheath progressively into the open distal end of the shaft, such that progressively proximal regions of the inner wall of the sheath transition through the transition zone to become part of the outer wall, and the proximal opening of the sheath moves distally along the implant.

\* \* \* \* \*