



US011011267B2

(12) **United States Patent**
Dixon et al.

(10) **Patent No.:** **US 11,011,267 B2**
(45) **Date of Patent:** ***May 18, 2021**

(54) **BED/ROOM/PATIENT ASSOCIATION SYSTEMS AND METHODS**

(71) Applicant: **Hill-Rom Services, Inc.**, Batesville, IN (US)

(72) Inventors: **Steven A. Dixon**, Cincinnati, OH (US); **Keith A. Huster**, Sunman, IN (US); **Michael A. Hood**, Batesville, IN (US); **James M. Allen**, Batesville, IN (US); **John D. Christie**, Batesville, IN (US); **Jack Barney Sing**, Batesville, IN (US); **Dan R. Tallent**, Hope, IN (US); **Umesh J. Rajani**, Cary, NC (US); **Clay G. Owsley**, Pittsboro, IN (US); **Thomas F. Heil**, Batesville, IN (US); **Richard Joseph Schuman, Sr.**, Cary, NC (US); **Timothy D. Wildman**, Metamora, IN (US)

(73) Assignee: **Hill-Rom Services, Inc.**, Batesville, IN (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 589 days.
This patent is subject to a terminal disclaimer.

(21) Appl. No.: **15/784,693**

(22) Filed: **Oct. 16, 2017**

(65) **Prior Publication Data**

US 2018/0039743 A1 Feb. 8, 2018

Related U.S. Application Data

(63) Continuation of application No. 14/487,279, filed on Sep. 16, 2014, now Pat. No. 9,830,424.
(Continued)

(51) **Int. Cl.**
A61G 7/05 (2006.01)
G16H 40/20 (2018.01)
G16H 40/67 (2018.01)

(52) **U.S. Cl.**
CPC *G16H 40/20* (2018.01); *A61G 7/05* (2013.01); *G16H 40/67* (2018.01)

(58) **Field of Classification Search**
CPC B60T 17/22; B60T 7/085; G06F 19/3406; G06F 19/3462
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,758,546 A 5/1930 Wartmann
2,330,356 A 9/1943 Belliveau
(Continued)

FOREIGN PATENT DOCUMENTS

EP 2031535 A2 3/2009
WO 2006/105269 A1 10/2006

OTHER PUBLICATIONS


Reference Manual, Laird WB45NBT, Version 1.0, revised Aug. 20, 2013, 37 pages.
(Continued)

Primary Examiner — Reginald R Reyes

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP

(57) **ABSTRACT**

Systems and methods of associating beds and/or rooms and/or patients are provided. One system and method involves using a signature of emitted light to determine a location of a patient bed in a healthcare facility. Another system and method involves reading a bar code from an array of redundant bar codes. Still another system and method involves manually entering location information on a graphical user interface of a patient bed for subsequent
(Continued)

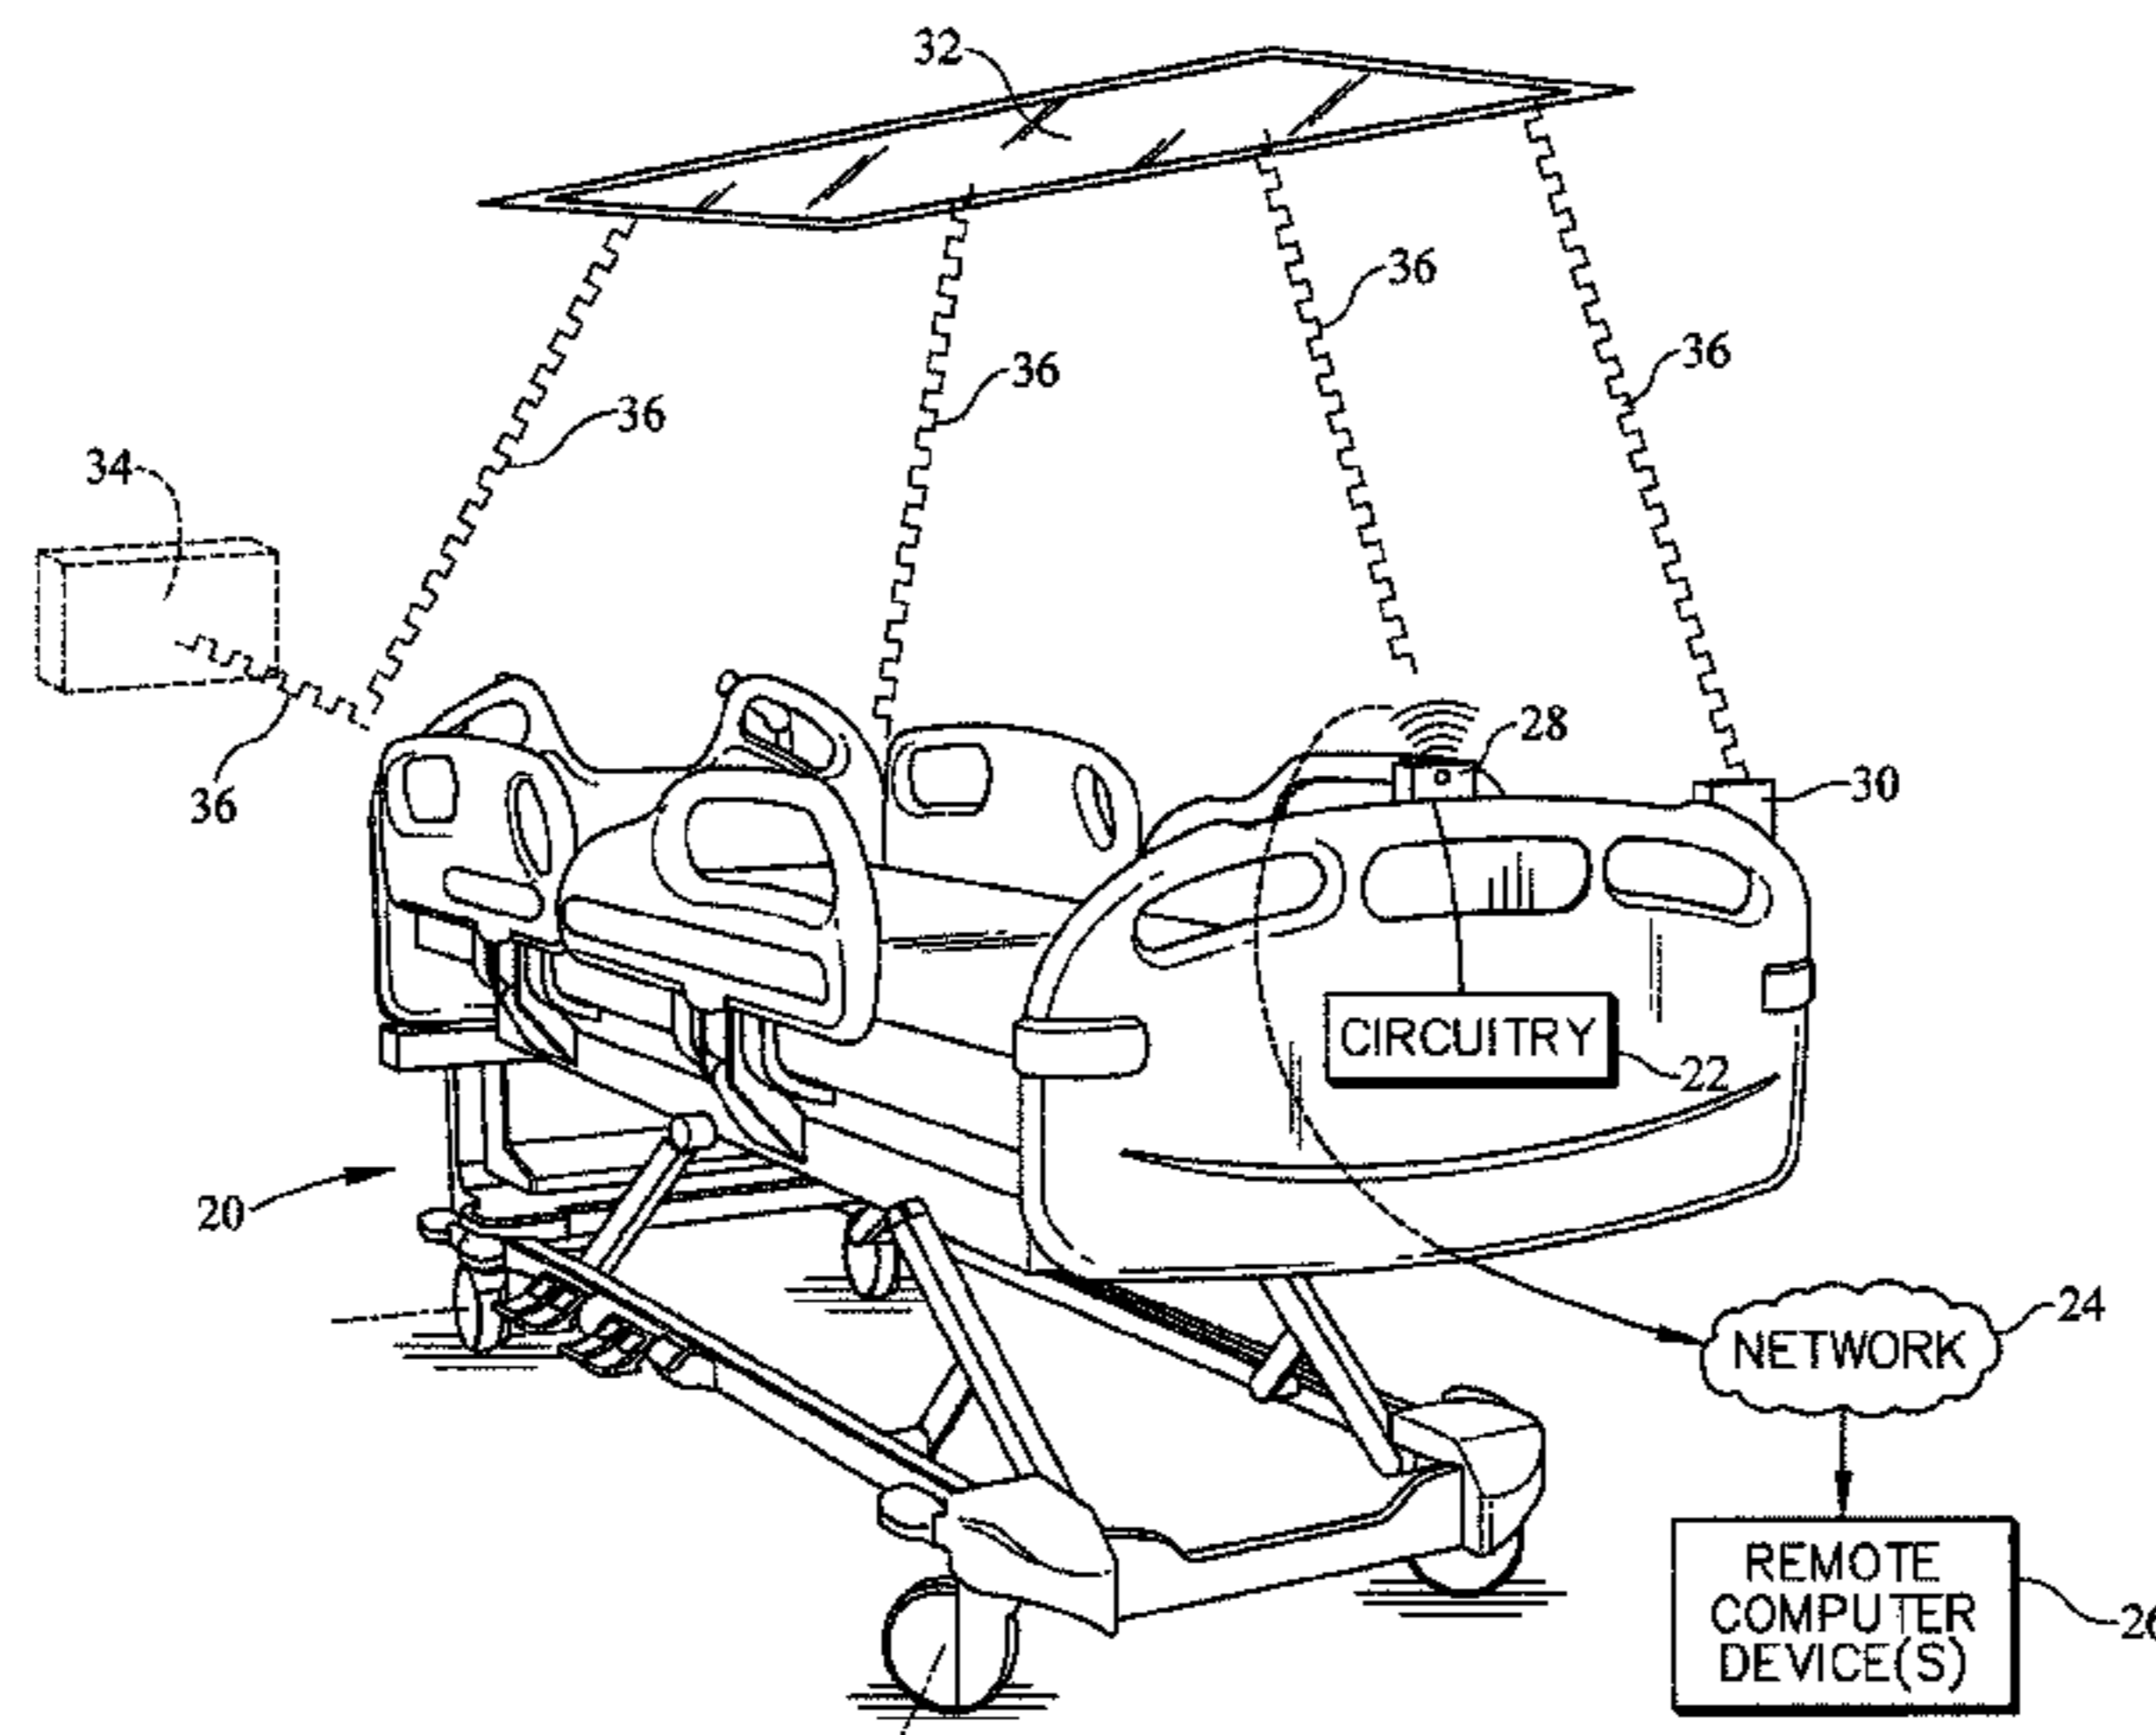

transmission. A further system and method involves sending bed ID and location ID along parallel paths from two independent circuits on a patient bed for receipt by two different transceivers and ultimately by two different remote computers that cooperate to associate the bed ID with the location ID. Still a further system and method involves using circuitry on a bed to mutate a received location ID and a bed ID into a single unique mutated ID such as by adding the location ID and bed ID and then performing a hashing operation.

19 Claims, 28 Drawing Sheets

Related U.S. Application Data

(60) Provisional application No. 61/879,399, filed on Sep. 18, 2013.

(56) References Cited

U.S. PATENT DOCUMENTS

2,335,524 A	11/1943	Lomax	4,578,671 A	3/1986	Flowers
2,736,888 A	2/1956	McLain	4,593,273 A	6/1986	Narcisse
2,896,021 A	7/1959	Philipps	4,598,275 A	7/1986	Ross et al.
D188,659 S	8/1960	Locke	4,601,064 A	7/1986	Shiple
3,054,201 A	9/1962	Burns	4,638,313 A	1/1987	Sherwood, Jr. et al.
3,098,220 A	7/1963	De Graaf	4,648,123 A	3/1987	Schrock
3,181,141 A	4/1965	Villiers	4,649,385 A	3/1987	Aires et al.
3,439,320 A	4/1969	Ward	4,654,629 A	3/1987	Bezos et al.
3,478,344 A	11/1969	Schwitzgebel et al.	4,663,625 A	5/1987	Yewen
3,553,383 A	1/1971	Rochtus	4,677,599 A	6/1987	Obayashi et al.
3,599,199 A	8/1971	Bunting	4,680,790 A	7/1987	Packard et al.
3,599,200 A	8/1971	Bunting	4,688,026 A	8/1987	Scribner et al.
3,659,586 A	5/1972	Johns et al.	4,699,149 A	10/1987	Rice
3,696,384 A	10/1972	Lester	4,706,689 A	11/1987	Man
3,739,329 A	6/1973	Lester	4,709,330 A	11/1987	Yokoi et al.
3,767,859 A	10/1973	Doering et al.	4,740,788 A	4/1988	Konneker
3,805,227 A	4/1974	Lester	4,748,668 A	5/1988	Shamir et al.
3,805,265 A	4/1974	Lester	4,752,951 A	6/1988	Konneker
3,810,136 A	5/1974	Lang et al.	4,792,798 A	12/1988	Wilowski
3,913,153 A	10/1975	Adams et al.	4,795,905 A	1/1989	Zierhut
3,973,200 A	8/1976	Åkerberg	4,803,599 A	2/1989	Trine et al.
4,052,567 A	10/1977	MacKay	4,814,751 A	3/1989	Hawkins et al.
4,067,005 A	1/1978	Levy et al.	4,833,452 A	5/1989	Currier
4,126,768 A	11/1978	Grenzow	4,833,467 A	5/1989	Kobayashi et al.
4,150,284 A	4/1979	Trenkler et al.	4,835,372 A	5/1989	Gombrich et al.
4,151,407 A	4/1979	McBride et al.	4,837,568 A	6/1989	Snaper
4,183,015 A	1/1980	Drew et al.	4,839,975 A	6/1989	Elmer
4,216,462 A	8/1980	McGrath et al.	4,843,640 A	6/1989	Juengel
4,224,596 A	9/1980	Knickel	4,849,615 A	7/1989	Mallet
4,225,953 A	9/1980	Simon et al.	4,853,692 A	8/1989	Wolk et al.
4,228,426 A	10/1980	Roberts	4,857,716 A	8/1989	Gombrich et al.
4,237,344 A	12/1980	Moore	4,862,088 A	8/1989	Etienne et al.
4,264,982 A	4/1981	Sakarya	4,871,997 A	10/1989	Adriaenssens et al.
4,275,385 A	6/1981	White	4,899,135 A	2/1990	Ghahariiran
4,279,433 A	7/1981	Petaja	4,947,152 A	8/1990	Hodges
4,298,863 A	11/1981	Natitus et al.	4,955,000 A	9/1990	Nastrom
4,331,953 A	5/1982	Blevins et al.	4,958,645 A	9/1990	Cadell et al.
4,356,475 A	10/1982	Neumann et al.	4,967,195 A	10/1990	Shiple
4,363,029 A	12/1982	Piliavin et al.	4,980,679 A	12/1990	Klaubert
4,363,137 A	12/1982	Salisbury	4,990,892 A	2/1991	Guest et al.
4,418,334 A	11/1983	Burnett	4,998,095 A	3/1991	Shields
4,455,548 A	6/1984	Burnett	4,998,939 A	3/1991	Potthast et al.
4,489,387 A	12/1984	Lamb et al.	5,005,005 A	4/1991	Brossia et al.
4,491,947 A	1/1985	Frank	5,006,830 A	4/1991	Merritt
4,495,495 A	1/1985	Ormanns et al.	5,014,040 A	5/1991	Weaver et al.
4,495,496 A	1/1985	Miller, III	5,027,314 A	6/1991	Linwood et al.
4,532,419 A	7/1985	Takeda	5,031,156 A	7/1991	Watts et al.
4,539,560 A	9/1985	Fleck et al.	5,041,086 A	8/1991	Koenig et al.
4,556,932 A	12/1985	Lehrer et al.	5,062,151 A	10/1991	Shiple
4,577,060 A	3/1986	Webb et al.	5,065,154 A	11/1991	Kaiser et al.
4,577,185 A	3/1986	Andersen	5,079,808 A	1/1992	Brown
			5,086,290 A	2/1992	Murray et al.
			5,103,108 A	4/1992	Crimmins
			5,119,104 A	6/1992	Heller
			5,124,991 A	6/1992	Allen
			5,131,040 A	7/1992	Knapczyk
			5,137,033 A	8/1992	Norton
			5,153,584 A	10/1992	Engira
			5,164,886 A	11/1992	Chang
			5,164,985 A	11/1992	Nysen et al.
			5,217,003 A	6/1993	Wilk
			5,231,273 A	7/1993	Caswell et al.
			5,266,944 A	11/1993	Carroll et al.
			5,274,311 A	12/1993	Littlejohn et al.
			5,276,496 A	1/1994	Heller et al.
			5,283,781 A	2/1994	Buda et al.
			5,291,399 A	3/1994	Chaco
			5,317,309 A	5/1994	Vercellotti et al.
			5,319,191 A	6/1994	Crimmins
			5,319,355 A	6/1994	Russek
			5,319,363 A	6/1994	Welch et al.
			5,334,851 A	8/1994	Good et al.
			5,339,259 A	8/1994	Puma et al.
			5,341,126 A	8/1994	Boykin
			5,351,149 A	9/1994	Crimmins
			5,355,222 A	10/1994	Heller et al.
			5,357,254 A	10/1994	Kah, Jr.
			5,363,425 A	11/1994	Mufti et al.
			5,375,604 A	12/1994	Kelly et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,387,993 A	2/1995	Heller et al.	5,792,063 A	8/1998	Danielsson et al.
5,396,224 A	3/1995	Dukes et al.	5,793,290 A	8/1998	Eagleson et al.
5,396,227 A	3/1995	Carroll et al.	5,808,564 A	9/1998	Simms et al.
5,402,469 A	3/1995	Hopper et al.	5,812,056 A	9/1998	Law
5,416,695 A	5/1995	Stutman et al.	5,822,418 A	10/1998	Yacenda et al.
5,421,177 A	6/1995	Sieber et al.	5,822,544 A	10/1998	Chaco et al.
5,434,775 A	7/1995	Sims et al.	5,828,306 A	10/1998	Curran
5,446,678 A	8/1995	Saltzstein et al.	5,831,533 A	11/1998	Kanno
RE35,035 E	9/1995	Shipley	5,838,223 A	11/1998	Gallant et al.
5,455,560 A	10/1995	Owen	5,838,472 A	11/1998	Welch et al.
5,455,851 A	10/1995	Chaco et al.	5,844,488 A	12/1998	Musick
5,458,123 A	10/1995	Unger	5,867,821 A	2/1999	Ballantyne et al.
5,461,390 A	10/1995	Hoshen	5,877,675 A	3/1999	Rebstock et al.
5,465,082 A	11/1995	Chaco	5,878,143 A	3/1999	Moore
5,471,404 A	11/1995	Mazer	5,897,506 A	4/1999	Cohn
5,475,367 A	12/1995	Prevost	5,898,459 A	4/1999	Smith et al.
5,482,036 A	1/1996	Diab et al.	5,910,776 A	6/1999	Black
5,515,426 A	5/1996	Yacenda et al.	5,933,488 A	8/1999	Marcus et al.
5,519,380 A	5/1996	Edwards	5,936,527 A	8/1999	Isaacman et al.
5,534,851 A	7/1996	Russek	5,936,539 A	8/1999	Fuchs
5,534,876 A	7/1996	Erickson et al.	5,942,986 A	8/1999	Shabot et al.
5,537,459 A	7/1996	Price et al.	5,944,659 A	8/1999	Flach et al.
5,548,637 A	8/1996	Heller et al.	5,956,660 A	9/1999	Neumann
5,549,113 A	8/1996	Halleck et al.	5,963,133 A	10/1999	Monjo
5,561,412 A	10/1996	Novak et al.	5,963,137 A	10/1999	Waters, Sr.
5,568,119 A	10/1996	Schipper et al.	5,973,598 A	10/1999	Beigel
5,572,195 A	11/1996	Heller et al.	5,974,389 A	10/1999	Clark et al.
5,576,952 A	11/1996	Stutman et al.	5,991,728 A	11/1999	DeBusk et al.
5,579,001 A	11/1996	Dempsey et al.	5,995,937 A	11/1999	DeBusk et al.
5,588,005 A	12/1996	Ali et al.	5,997,476 A	12/1999	Brown
5,594,786 A	1/1997	Chaco et al.	RE36,530 E	1/2000	Heller et al.
5,621,388 A	4/1997	Sherburne et al.	6,014,633 A	1/2000	DeBusk et al.
5,627,524 A	5/1997	Fredrickson et al.	6,026,818 A	2/2000	Blair et al.
5,629,678 A	5/1997	Gargano et al.	6,028,514 A	2/2000	Lemelson et al.
5,633,742 A	5/1997	Shipley	6,031,458 A	2/2000	Jacobsen et al.
5,635,907 A	6/1997	Bernard et al.	6,031,459 A	2/2000	Lake
5,636,245 A	6/1997	Ernst et al.	6,031,460 A	2/2000	Banks
5,639,393 A	6/1997	Veltum et al.	6,034,603 A	3/2000	Steeves
5,640,002 A	6/1997	Ruppert et al.	6,034,622 A	3/2000	Levine
5,640,146 A	6/1997	Campana, Jr.	6,037,879 A	3/2000	Tuttle
5,640,953 A	6/1997	Bishop et al.	6,040,773 A	3/2000	Vega et al.
5,650,769 A	7/1997	Campana, Jr.	6,049,278 A	4/2000	Guthrie et al.
5,650,770 A	7/1997	Schlager et al.	6,049,290 A	4/2000	Halstead
5,661,457 A	8/1997	Ghaffari et al.	6,052,710 A	4/2000	Saliba et al.
5,664,035 A	9/1997	Tsuji et al.	6,054,927 A	4/2000	Brickell
5,664,270 A	9/1997	Bell et al.	6,055,487 A	4/2000	Margery et al.
5,682,139 A	10/1997	Pradeep et al.	6,055,506 A	4/2000	Frasca, Jr.
5,686,888 A	11/1997	Welles, II et al.	6,057,758 A	5/2000	Dempsey et al.
5,686,902 A	11/1997	Reis et al.	6,057,782 A	5/2000	Koenig
5,687,109 A	11/1997	Protigal et al.	6,067,019 A	5/2000	Scott
5,687,735 A	11/1997	Dempsey et al.	6,069,555 A	5/2000	Skitek et al.
5,689,229 A	11/1997	Chaco et al.	6,069,564 A	5/2000	Hatano et al.
5,691,980 A	11/1997	Welles, II et al.	6,069,570 A	5/2000	Herring
5,699,038 A	12/1997	Ulrich et al.	6,075,707 A	6/2000	Ferguson et al.
5,705,980 A	1/1998	Shapiro	6,076,166 A	6/2000	Moshfeghi et al.
5,708,421 A	1/1998	Boyd	6,078,251 A	6/2000	Landt et al.
5,708,423 A	1/1998	Ghaffari et al.	6,078,259 A	6/2000	Brady et al.
5,713,856 A	2/1998	Eggers et al.	6,078,261 A	6/2000	Davsko
5,719,761 A	2/1998	Gatti et al.	6,078,631 A	6/2000	Yabe et al.
5,731,757 A	3/1998	Layson, Jr.	RE36,791 E	7/2000	Heller
5,742,237 A	4/1998	Bledsoe	6,084,512 A	7/2000	Elberty et al.
5,742,238 A	4/1998	Fox	6,085,069 A	7/2000	Sharpe
5,745,037 A	4/1998	Guthrie et al.	6,085,493 A	7/2000	DeBusk et al.
5,748,148 A	5/1998	Heiser et al.	6,088,362 A	7/2000	Turnbull et al.
5,751,246 A	5/1998	Hertel	6,091,332 A	7/2000	Eberhardt et al.
5,752,917 A	5/1998	Fuchs	6,091,530 A	7/2000	Duckworth
5,754,125 A	5/1998	Pearce	6,093,146 A	7/2000	Filangeri
5,760,704 A	6/1998	Barton et al.	6,097,301 A	8/2000	Tuttle
5,764,162 A	6/1998	Ehrlich	6,097,308 A	8/2000	Albert et al.
5,767,788 A	6/1998	Ness	6,100,804 A	8/2000	Brady et al.
5,767,791 A	6/1998	Stoop et al.	6,101,390 A	8/2000	Jayaraman et al.
5,771,003 A	6/1998	Seymour	6,104,295 A	8/2000	Gaisser et al.
5,776,056 A	7/1998	Bu et al.	6,104,311 A	8/2000	Lastinger
5,781,442 A	7/1998	Engleson et al.	6,111,506 A	8/2000	Yap et al.
5,781,632 A	7/1998	Odom	6,114,962 A	9/2000	Wiklof et al.
			6,118,379 A	9/2000	Kodukula et al.
			6,127,928 A	10/2000	Issacman et al.
			6,130,612 A	10/2000	Castellano et al.
			6,133,832 A	10/2000	Winder et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,133,837	A	10/2000	Riley	6,529,164	B1	3/2003	Carter
6,137,411	A	10/2000	Tyren	6,533,453	B1	3/2003	Heidsieck et al.
6,137,412	A	10/2000	Herzer	6,535,576	B2	3/2003	Vafi et al.
6,137,414	A	10/2000	Federman	6,544,174	B2	4/2003	West et al.
6,144,301	A	11/2000	Frieden	6,551,243	B2	4/2003	Bocioneck et al.
6,144,303	A	11/2000	Federman	6,553,106	B1	4/2003	Gould et al.
6,147,592	A	11/2000	Ulrich et al.	6,554,174	B1	4/2003	Aceves
6,148,291	A	11/2000	Radican	6,556,630	B1	4/2003	Brinsfield et al.
6,150,948	A	11/2000	Watkins	6,560,274	B1	5/2003	Leitgeb et al.
6,150,950	A	11/2000	Shen Liu	6,572,556	B2	6/2003	Stoycos et al.
6,154,135	A	11/2000	Kane et al.	6,575,901	B2	6/2003	Stoycos et al.
6,154,139	A	11/2000	Heller	6,581,204	B2	6/2003	DeBusk et al.
6,157,302	A	12/2000	Kolton et al.	6,584,182	B2	6/2003	Brodnick
6,160,881	A	12/2000	Beyda et al.	6,584,454	B1	6/2003	Hummel, Jr. et al.
6,169,484	B1	1/2001	Schuchman et al.	6,585,645	B2	7/2003	Hutchinson
6,169,485	B1	1/2001	Campana, Jr.	6,589,170	B1	7/2003	Flach et al.
6,177,861	B1	1/2001	MacLellan et al.	6,593,528	B2	7/2003	Franklin-Lees et al.
6,183,417	B1	2/2001	Geheb et al.	6,593,845	B1	7/2003	Friedman et al.
6,203,495	B1	3/2001	Bardy	6,594,146	B2	7/2003	Frangesch et al.
6,204,765	B1	3/2001	Brady et al.	6,594,519	B2	7/2003	Stoycos et al.
6,204,813	B1	3/2001	Wadell et al.	6,600,418	B2	7/2003	Francis et al.
6,208,250	B1	3/2001	Dixon et al.	6,600,421	B2	7/2003	Freeman
6,211,666	B1	4/2001	Acker	6,603,494	B1	8/2003	Banks et al.
6,211,781	B1	4/2001	McDonald	6,609,115	B1	8/2003	Mehring et al.
6,211,796	B1	4/2001	Toms et al.	6,616,606	B1	9/2003	Petersen et al.
6,215,389	B1	4/2001	Schmidt	6,622,088	B2	9/2003	Hood
6,222,440	B1	4/2001	Heller	6,640,246	B1	10/2003	Gary, Jr. et al.
6,228,029	B1	5/2001	Eccardt et al.	6,643,238	B2	11/2003	Nakajima
6,236,319	B1	5/2001	Pitzer et al.	6,650,346	B1	11/2003	Jaeger et al.
6,241,668	B1	6/2001	Herzog	6,659,947	B1	12/2003	Carter et al.
6,249,234	B1	6/2001	Ely et al.	6,665,385	B2	12/2003	Rogers et al.
6,259,355	B1	7/2001	Chaco et al.	6,665,820	B1	12/2003	Frowein et al.
6,262,666	B1	7/2001	Lodichand	6,669,630	B1	12/2003	Joliat et al.
6,264,614	B1	7/2001	Albert et al.	6,671,547	B2	12/2003	Lyster et al.
6,268,797	B1	7/2001	Berube et al.	6,671,563	B1	12/2003	Engelson et al.
6,275,153	B1	8/2001	Brooks	6,685,633	B2	2/2004	Albert et al.
6,279,183	B1	8/2001	Kummer et al.	6,689,091	B2	2/2004	Bui et al.
6,280,409	B1	8/2001	Stone et al.	6,693,513	B2	2/2004	Tuttle
6,285,742	B1	9/2001	Haumann et al.	6,693,514	B2	2/2004	Perea, Jr. et al.
6,287,253	B1	9/2001	Ortega et al.	6,694,367	B1	2/2004	Miesbauer et al.
6,289,237	B1	9/2001	Mickle et al.	6,694,509	B1	2/2004	Stoval et al.
6,293,699	B1	9/2001	Bailey et al.	6,697,765	B2	2/2004	Kuth
6,294,953	B1	9/2001	Steeves	6,707,476	B1	3/2004	Hochstedler
6,302,844	B1	10/2001	Walker et al.	6,714,913	B2	3/2004	Brandt et al.
6,314,556	B1	11/2001	DeBusk et al.	6,721,818	B1	4/2004	Nakamura
6,320,510	B2	11/2001	Menkedick et al.	6,726,634	B2	4/2004	Freeman
6,333,690	B1	12/2001	Nelson et al.	6,727,818	B1	4/2004	Wildman et al.
6,343,064	B1	1/2002	Jabbarnezhad	6,731,311	B2	5/2004	Bufe et al.
6,344,794	B1	2/2002	Ulrich et al.	6,731,908	B2	5/2004	Berliner et al.
6,348,777	B1	2/2002	Brown et al.	6,731,989	B2	5/2004	Engleson et al.
6,353,413	B1	3/2002	White et al.	6,740,033	B1	5/2004	Olejniczak et al.
6,362,725	B1	3/2002	Ulrich et al.	6,747,560	B2	6/2004	Stevens, III
6,364,834	B1	4/2002	Reuss et al.	6,747,562	B2	6/2004	Giraldin et al.
6,398,727	B1	6/2002	Bui et al.	6,749,566	B2	6/2004	Russ
6,400,956	B1	6/2002	Richton	6,751,630	B1	6/2004	Franks et al.
6,406,426	B1	6/2002	Reuss et al.	6,754,545	B2	6/2004	Haeuser et al.
6,407,335	B1	6/2002	Franklin-Lees et al.	6,754,883	B2	6/2004	DeBusk et al.
6,412,980	B1	7/2002	Lounsberry et al.	6,756,918	B2	6/2004	Fomukong
6,416,471	B1	7/2002	Kumar et al.	6,759,959	B2	7/2004	Wildman
6,418,416	B1	7/2002	Rosenberg et al.	6,763,541	B2	7/2004	Mahoney et al.
6,421,649	B1	7/2002	Rattner	6,771,172	B1	8/2004	Robinson et al.
6,424,264	B1	7/2002	Giraldin et al.	6,773,396	B2	8/2004	Flach et al.
6,439,769	B1	8/2002	Polkus et al.	6,778,225	B2	8/2004	David
6,441,742	B1	8/2002	Lovely et al.	6,781,517	B2	8/2004	Moster et al.
6,442,290	B1	8/2002	Ellis et al.	6,784,797	B2	8/2004	Smith et al.
6,445,299	B1	9/2002	Rojas, Jr.	6,791,460	B2	9/2004	Dixon et al.
6,450,956	B1	9/2002	Rappaport et al.	6,792,396	B2	9/2004	Inda et al.
6,462,656	B2	10/2002	Ulrich et al.	6,798,533	B2	9/2004	Tipirneni
6,486,792	B1	11/2002	Moster et al.	6,801,227	B2	10/2004	Bocioneck et al.
6,486,794	B1	11/2002	Calistro et al.	6,807,543	B2	10/2004	Muthya
6,493,568	B1	12/2002	Bell et al.	6,812,824	B1	11/2004	Goldinger et al.
6,494,831	B1	12/2002	Koritzinsky	6,825,763	B2	11/2004	Ulrich et al.
6,510,344	B1	1/2003	Halpern	6,826,578	B2	11/2004	Brackett et al.
6,516,324	B1	2/2003	Jones et al.	6,828,992	B1	12/2004	Freeman et al.
6,526,310	B1	2/2003	Carter et al.	6,829,796	B2	12/2004	Salvatini et al.
				6,830,549	B2	12/2004	Bui et al.
				6,832,199	B1	12/2004	Kucek et al.
				6,838,992	B2	1/2005	Tenarvitz
				6,840,117	B2	1/2005	Hubbard, Jr.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,843,415 B2	1/2005	Vogler	7,164,354 B1	1/2007	Panzer
6,847,435 B2	1/2005	Honda et al.	7,165,040 B2	1/2007	Ehrman et al.
6,847,814 B1	1/2005	Vogeleisen	7,167,095 B2	1/2007	Carrender
6,859,761 B2	2/2005	Bensky et al.	7,170,407 B2	1/2007	Wagner
6,868,256 B2	3/2005	Dooley et al.	7,174,172 B2	2/2007	Sharony et al.
6,871,211 B2	3/2005	Labounty et al.	7,190,778 B2	3/2007	Kucmerowski
6,873,884 B2	3/2005	Brackett et al.	7,196,621 B2	3/2007	Kochis
6,876,303 B2	4/2005	Reeder et al.	7,199,716 B2	4/2007	Shanks et al.
6,876,985 B2	4/2005	Kawanaka	7,202,785 B2	4/2007	Maloney
6,884,255 B1	4/2005	Newton	7,203,690 B2	4/2007	Braun et al.
6,885,288 B2	4/2005	Pincus	7,209,790 B2	4/2007	Thompson et al.
6,891,909 B2	5/2005	Hurley et al.	7,218,231 B2	5/2007	Higham
6,897,780 B2	5/2005	Ulrich et al.	7,225,241 B2	5/2007	Yada
6,904,161 B1	6/2005	Becker et al.	7,230,536 B2	6/2007	Shinada et al.
6,909,995 B2	6/2005	Shiraishi	7,242,306 B2	7/2007	Wildman et al.
6,912,549 B2	6/2005	Rotter et al.	7,242,308 B2	7/2007	Ulrich et al.
6,915,170 B2	7/2005	Engleson et al.	7,248,880 B2	7/2007	Gheorghiu et al.
6,925,367 B2	8/2005	Fontius	7,248,933 B2	7/2007	Wildman
6,930,878 B2	8/2005	Brackett et al.	7,259,676 B2	8/2007	Knadle, Jr. et al.
6,954,148 B2	10/2005	Pulkkinen et al.	7,265,668 B1	9/2007	Brosius
6,958,706 B2	10/2005	Chaco et al.	7,269,427 B2	9/2007	Hector et al.
6,968,194 B2	11/2005	Aljadeff et al.	7,277,048 B2	10/2007	Hessing
6,972,682 B2	12/2005	Lareau et al.	7,277,889 B2	10/2007	Addonisio et al.
6,988,989 B2	1/2006	Weiner et al.	7,283,046 B2	10/2007	Culpepper et al.
6,998,985 B2	2/2006	Reisman et al.	7,283,423 B2	10/2007	Holm et al.
6,998,986 B2	2/2006	Smith	7,286,868 B2	10/2007	Govari
7,002,468 B2	2/2006	Eveland et al.	7,292,151 B2	11/2007	Ferguson et al.
7,003,443 B2	2/2006	Ford et al.	7,295,115 B2	11/2007	Aljadeff et al.
7,005,980 B1	2/2006	Schmidt et al.	7,295,132 B2	11/2007	Steiner
7,009,495 B2	3/2006	Hughes et al.	7,298,359 B2	11/2007	Kim et al.
7,009,516 B2	3/2006	Enea	7,301,451 B2	11/2007	Hastings
7,014,100 B2	3/2006	Zierolf	7,304,577 B2	12/2007	Waldner et al.
7,019,663 B2	3/2006	Sharony	7,304,578 B1	12/2007	Sayers et al.
7,030,761 B2	4/2006	Bridgelall et al.	7,304,579 B2	12/2007	Diorio et al.
7,030,811 B2	4/2006	Goren et al.	7,307,522 B2	12/2007	Dawson
7,034,684 B2	4/2006	Boman et al.	7,313,403 B2	12/2007	Gong et al.
7,034,690 B2	4/2006	Chaco	7,315,248 B2	1/2008	Egbert
7,035,818 B1	4/2006	Bandy et al.	7,315,281 B2	1/2008	Dejanovic et al.
7,038,573 B2	5/2006	Bann	7,319,386 B2	1/2008	Collins, Jr. et al.
7,038,584 B2	5/2006	Carter	7,319,395 B2	1/2008	Puzio et al.
7,038,588 B2	5/2006	Boone et al.	7,319,397 B2	1/2008	Chung et al.
7,038,589 B2	5/2006	Schmidt et al.	7,319,412 B1	1/2008	Coppinger et al.
7,042,358 B2	5/2006	Moore	7,321,305 B2	1/2008	Göllü
7,042,361 B2	5/2006	Kazdin et al.	7,333,018 B2	2/2008	Singh et al.
7,044,387 B2	5/2006	Becker et al.	7,336,187 B2	2/2008	Hubbard, Jr. et al.
7,046,153 B2	5/2006	Oja et al.	7,336,563 B2	2/2008	Holm
7,046,162 B2	5/2006	Dunstan	7,339,477 B2	3/2008	Puzio et al.
7,049,594 B2	5/2006	Wu et al.	7,339,479 B2	3/2008	Nishimura
7,053,779 B2	5/2006	Thompson	7,362,656 B2	4/2008	Holm
7,053,781 B1	5/2006	Haire et al.	7,370,808 B2	5/2008	Eastin
7,053,831 B2	5/2006	Dempsey et al.	7,375,648 B1	5/2008	Mulka et al.
7,056,289 B2	6/2006	Kasper et al.	7,375,654 B2	5/2008	Culpepper et al.
7,057,509 B2	6/2006	Gualdi et al.	7,376,123 B2	5/2008	Reuss
7,061,366 B2	6/2006	Bell et al.	7,394,385 B2	7/2008	Franco, Jr. et al.
7,061,384 B2	6/2006	Fujimoto	7,411,509 B2	8/2008	Rosenfeld et al.
7,062,455 B1	6/2006	Tobey	7,415,212 B2	8/2008	Matsushita et al.
7,068,143 B2	6/2006	Doering et al.	7,417,544 B2	8/2008	Artem et al.
7,071,820 B2	7/2006	Callaway	7,443,299 B2	10/2008	Forster
7,071,843 B2	7/2006	Hashida et al.	7,446,664 B2	11/2008	White
7,075,438 B2	7/2006	Kent et al.	7,473,097 B2	1/2009	Raby et al.
7,080,061 B2	7/2006	Kabala	7,474,224 B2	1/2009	Long et al.
7,084,740 B2	8/2006	Bridgelall	7,515,044 B2	4/2009	Welch et al.
7,091,879 B2	8/2006	Swetlik et al.	7,518,502 B2	4/2009	Austin et al.
7,092,376 B2	8/2006	Schuman	7,538,679 B2	5/2009	Shanks
7,099,895 B2	8/2006	Dempsey	7,541,927 B2	6/2009	Dupler et al.
7,102,510 B2	9/2006	Boling et al.	7,551,083 B2	6/2009	Modes et al.
7,106,189 B2	9/2006	Burneske et al.	7,567,794 B2	7/2009	Dempsey
7,116,230 B2	10/2006	Klowak	7,598,853 B2	10/2009	Becker et al.
7,117,027 B2	10/2006	Zheng et al.	7,623,250 B2	11/2009	Moctezuma de la Barrera et al.
7,138,913 B2	11/2006	Mackenzie et al.	7,627,334 B2	12/2009	Cohen et al.
7,142,112 B2	11/2006	Buckingham et al.	7,664,686 B2	2/2010	Czyszczeński et al.
7,151,455 B2	12/2006	Lindsay et al.	7,667,572 B2	2/2010	Husak et al.
7,152,791 B2	12/2006	Chappidi et al.	7,714,728 B2	5/2010	Koblasz
7,154,397 B2	12/2006	Zerhusen et al.	7,724,147 B2	5/2010	Brown
7,158,030 B2	1/2007	Chung	7,725,195 B2	5/2010	Lima et al.
			7,734,476 B2	6/2010	Wildman et al.
			7,737,850 B2	6/2010	Malik
			7,750,793 B2	7/2010	Juels
			7,755,541 B2	7/2010	Wisherd et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,756,723 B2 7/2010 Rosow et al.
 7,761,320 B2 7/2010 Fliess et al.
 7,765,286 B2 7/2010 Mark
 7,800,914 B2 9/2010 Dully
 7,844,505 B1 11/2010 Arneson et al.
 7,848,760 B2 12/2010 Caspi et al.
 7,869,861 B2 1/2011 Moctezuma de la Barrera et al.
 7,890,349 B2 2/2011 Cole et al.
 7,893,842 B2 2/2011 Deutsch
 7,907,053 B2 3/2011 Wildman et al.
 7,916,023 B2 3/2011 Rado
 7,920,050 B2 4/2011 Juels et al.
 7,928,844 B2 4/2011 Mackenzie et al.
 7,933,780 B2 4/2011 De La Huerga
 7,958,087 B2 6/2011 Blumenau
 7,966,008 B2 6/2011 Graves et al.
 8,026,821 B2 9/2011 Reeder et al.
 8,031,057 B2 10/2011 McNeely et al.
 8,073,558 B2 12/2011 Koch et al.
 8,102,254 B2 1/2012 Becker et al.
 8,160,677 B2 4/2012 Gielen et al.
 8,164,444 B2 4/2012 Anderson et al.
 8,190,730 B2 5/2012 Dempsey
 8,223,009 B2 7/2012 Anderson et al.
 8,248,467 B1 8/2012 Ganick et al.
 8,272,892 B2 9/2012 McNeely et al.
 8,284,047 B2 10/2012 Collins, Jr. et al.
 8,310,364 B2 11/2012 Derks et al.
 8,319,633 B2 11/2012 Becker et al.
 8,321,302 B2 11/2012 Bauer et al.
 8,334,898 B1 12/2012 Ryan et al.
 8,334,901 B1 12/2012 Ganick et al.
 8,390,462 B2 3/2013 Belz et al.
 8,416,072 B2 4/2013 Tenarvitz
 8,416,290 B2 4/2013 Ryan et al.
 8,432,438 B2 4/2013 Ryan et al.
 8,436,896 B2 5/2013 Staats et al.
 8,447,626 B2 5/2013 Sun et al.
 8,457,502 B2 6/2013 Ryan et al.
 8,461,968 B2 6/2013 Ball et al.
 8,461,982 B2 6/2013 Becker et al.
 8,514,071 B2 8/2013 Derks et al.
 8,516,514 B2 8/2013 Belz et al.
 8,519,823 B2 8/2013 Rinkes
 8,520,065 B2 8/2013 Staats et al.
 8,558,660 B2 10/2013 Nix et al.
 8,604,916 B2 12/2013 McNeely et al.
 8,604,917 B2 12/2013 Collins et al.
 8,610,562 B2 12/2013 Weiner et al.
 8,650,045 B2 2/2014 Baldock et al.
 8,674,826 B2 3/2014 Becker et al.
 8,689,376 B2 4/2014 Becker et al.
 8,752,045 B2 6/2014 Fitzgerald et al.
 8,781,847 B2 7/2014 Simms et al.
 9,020,963 B2 4/2015 Goodman et al.
 9,026,301 B2 5/2015 Zini et al.
 9,830,424 B2 11/2017 Dixon et al.
 2001/0050610 A1 12/2001 Gelston
 2001/0051765 A1 12/2001 Walker et al.
 2002/0044059 A1 4/2002 Reeder et al.
 2002/0067273 A1 6/2002 Jaques et al.
 2002/0070867 A1 6/2002 Conway et al.
 2002/0165733 A1 11/2002 Pulkkinen et al.
 2002/0173286 A1 11/2002 Lindoff et al.
 2002/0173991 A1 11/2002 Avitall
 2003/0010345 A1 1/2003 Koblasz et al.
 2003/0028449 A1 2/2003 Heinen et al.
 2003/0132845 A1 7/2003 McDaniel, III
 2003/0149598 A1 8/2003 Santoso et al.
 2003/0176798 A1 9/2003 Simon
 2004/0024660 A1 2/2004 Ganesh et al.
 2004/0106854 A1 6/2004 Muraki

2004/0186358 A1 9/2004 Chernow et al.
 2005/0071198 A1 3/2005 Krupa
 2005/0122119 A1 6/2005 Barlow
 2005/0131729 A1 6/2005 Melby et al.
 2006/0012474 A1 1/2006 Lu et al.
 2006/0022818 A1 2/2006 Piltonen
 2006/0028336 A1 2/2006 Glenn et al.
 2006/0031259 A1 2/2006 Gibson et al.
 2006/0038676 A1 2/2006 Richards
 2006/0071774 A1 4/2006 Brown et al.
 2006/0082444 A1 4/2006 Sweeney, II et al.
 2006/0097863 A1 5/2006 Horowitz et al.
 2006/0135083 A1 6/2006 Leinonen et al.
 2006/0161214 A1 7/2006 Patel
 2006/0220798 A1 10/2006 Willis
 2006/0253590 A1 11/2006 Nagy et al.
 2007/0005558 A1 1/2007 Canfield
 2007/0015960 A1 1/2007 Gornert et al.
 2007/0033072 A1 2/2007 Bildirici
 2007/0073116 A1 3/2007 Kiani et al.
 2007/0093879 A1 4/2007 Bek et al.
 2007/0123173 A1 5/2007 Stobbe
 2007/0129967 A1 6/2007 Thompson et al.
 2007/0157385 A1* 7/2007 Lemire A61G 7/0509
 5/600
 2007/0210917 A1 9/2007 Collins, Jr. et al.
 2007/0271122 A1 11/2007 Zaleski
 2008/0004993 A1 1/2008 Horspool et al.
 2008/0026713 A1 1/2008 Sekhar et al.
 2008/0040244 A1 2/2008 Ricciuti et al.
 2008/0100706 A1 5/2008 Breed
 2008/0106418 A1 5/2008 Sloan et al.
 2008/0108372 A1 5/2008 Breed
 2008/0126125 A1 5/2008 Lichtenstein et al.
 2008/0126126 A1 5/2008 Ballai
 2008/0136621 A1 6/2008 Malik et al.
 2008/0136635 A1 6/2008 Malik
 2008/0140544 A1 6/2008 Ehrman et al.
 2008/0180322 A1 7/2008 Islam et al.
 2008/0201388 A1 8/2008 Wood et al.
 2008/0215360 A1 9/2008 Dicks et al.
 2008/0238676 A1 10/2008 Dhillon et al.
 2008/0242945 A1 10/2008 Gugliotti et al.
 2008/0300918 A1 12/2008 Tenenbaum et al.
 2008/0312974 A2 12/2008 Rosow et al.
 2008/0312975 A2 12/2008 Rosow et al.
 2009/0018882 A1 1/2009 Burton et al.
 2009/0033500 A1 2/2009 Malik et al.
 2009/0079549 A1 3/2009 Ruder
 2009/0300507 A1 12/2009 Raghavan et al.
 2010/0001838 A1 1/2010 Miodownik et al.
 2010/0217618 A1 8/2010 Piccirillo et al.
 2010/0289885 A1 11/2010 Lu et al.
 2011/0050411 A1 3/2011 Schuman et al.
 2011/0125513 A1 5/2011 Tenarvitz et al.
 2011/0125524 A1 5/2011 Tenarvitz et al.
 2011/0208541 A1 8/2011 Wilson et al.
 2011/0227740 A1 9/2011 Wohltjen
 2012/0316892 A1* 12/2012 Huster G16H 40/20
 705/2
 2013/0069771 A1 3/2013 Frondorf
 2014/0207490 A1* 7/2014 Shindo G16H 20/70
 705/3
 2015/0081335 A1 3/2015 Dixon et al.

OTHER PUBLICATIONS

EP Search Report for Application No. EP 14185232.7-1952, dated Mar. 16, 2015, 6 pages.
 Summons to Attend Oral Proceedings issued by the European Patent Office for European Patent Application No. 14185232.7; dated Nov. 13, 2020 (9 pages).

* cited by examiner

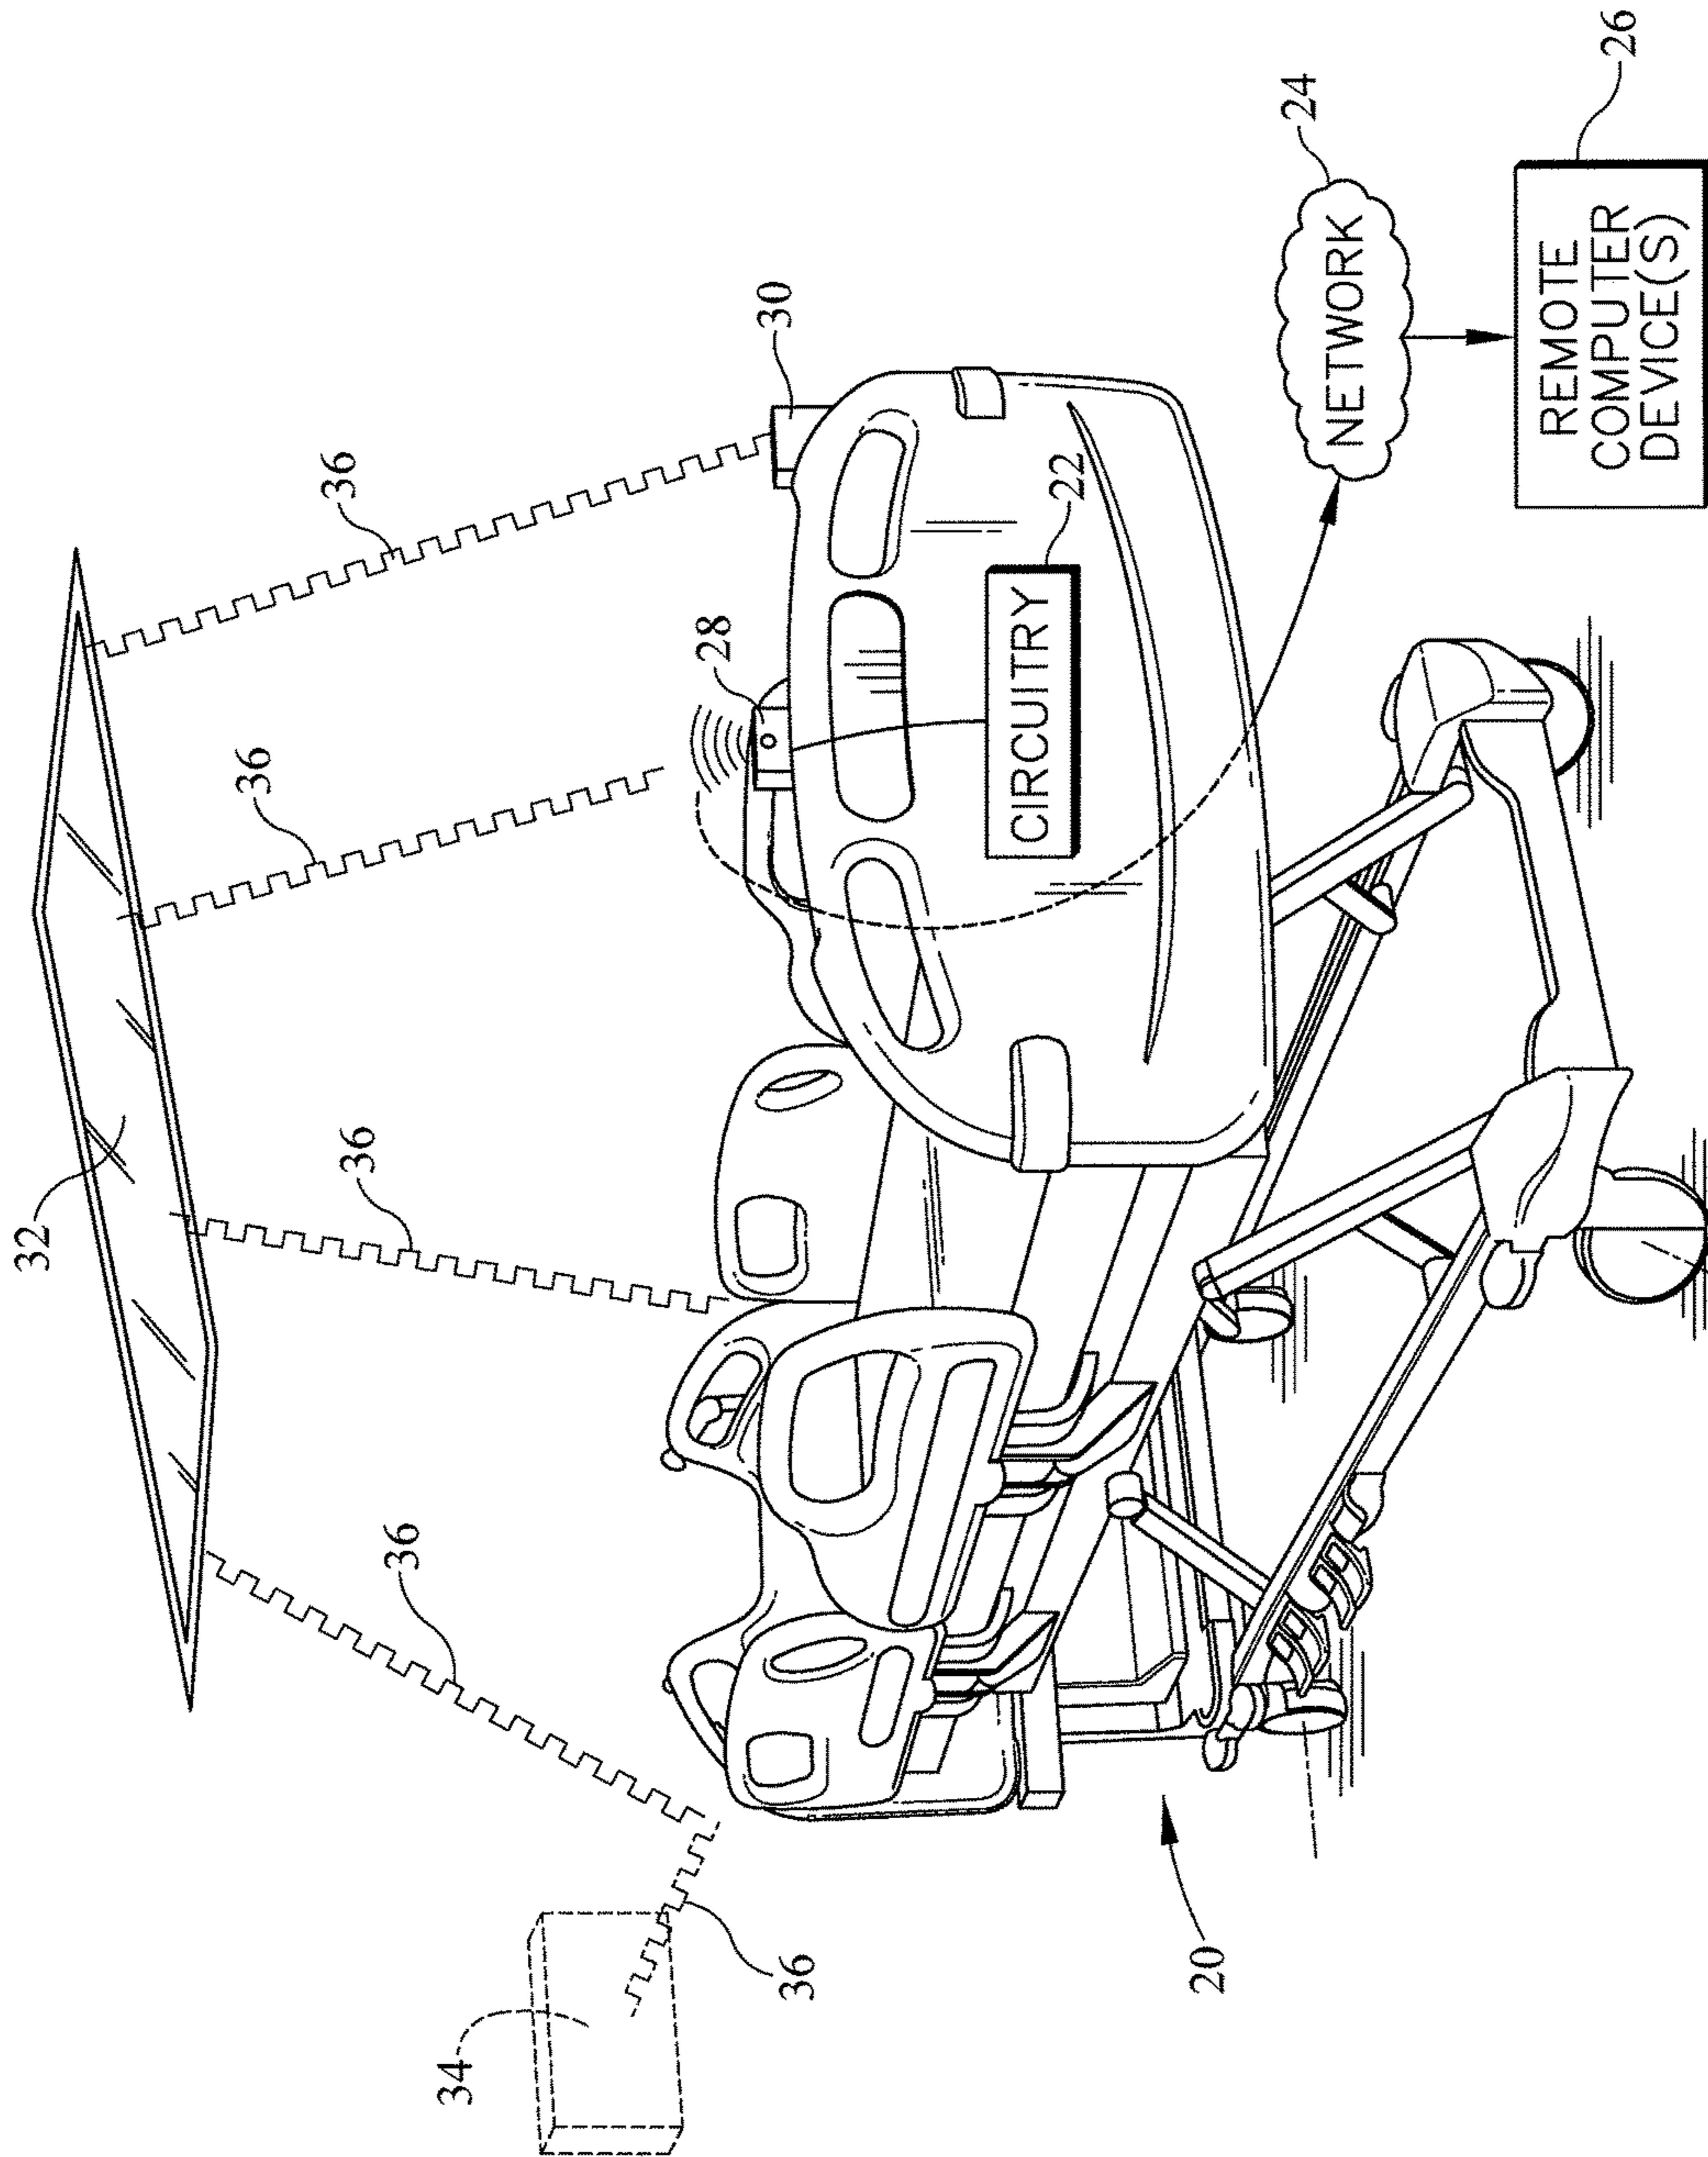


FIG. 1

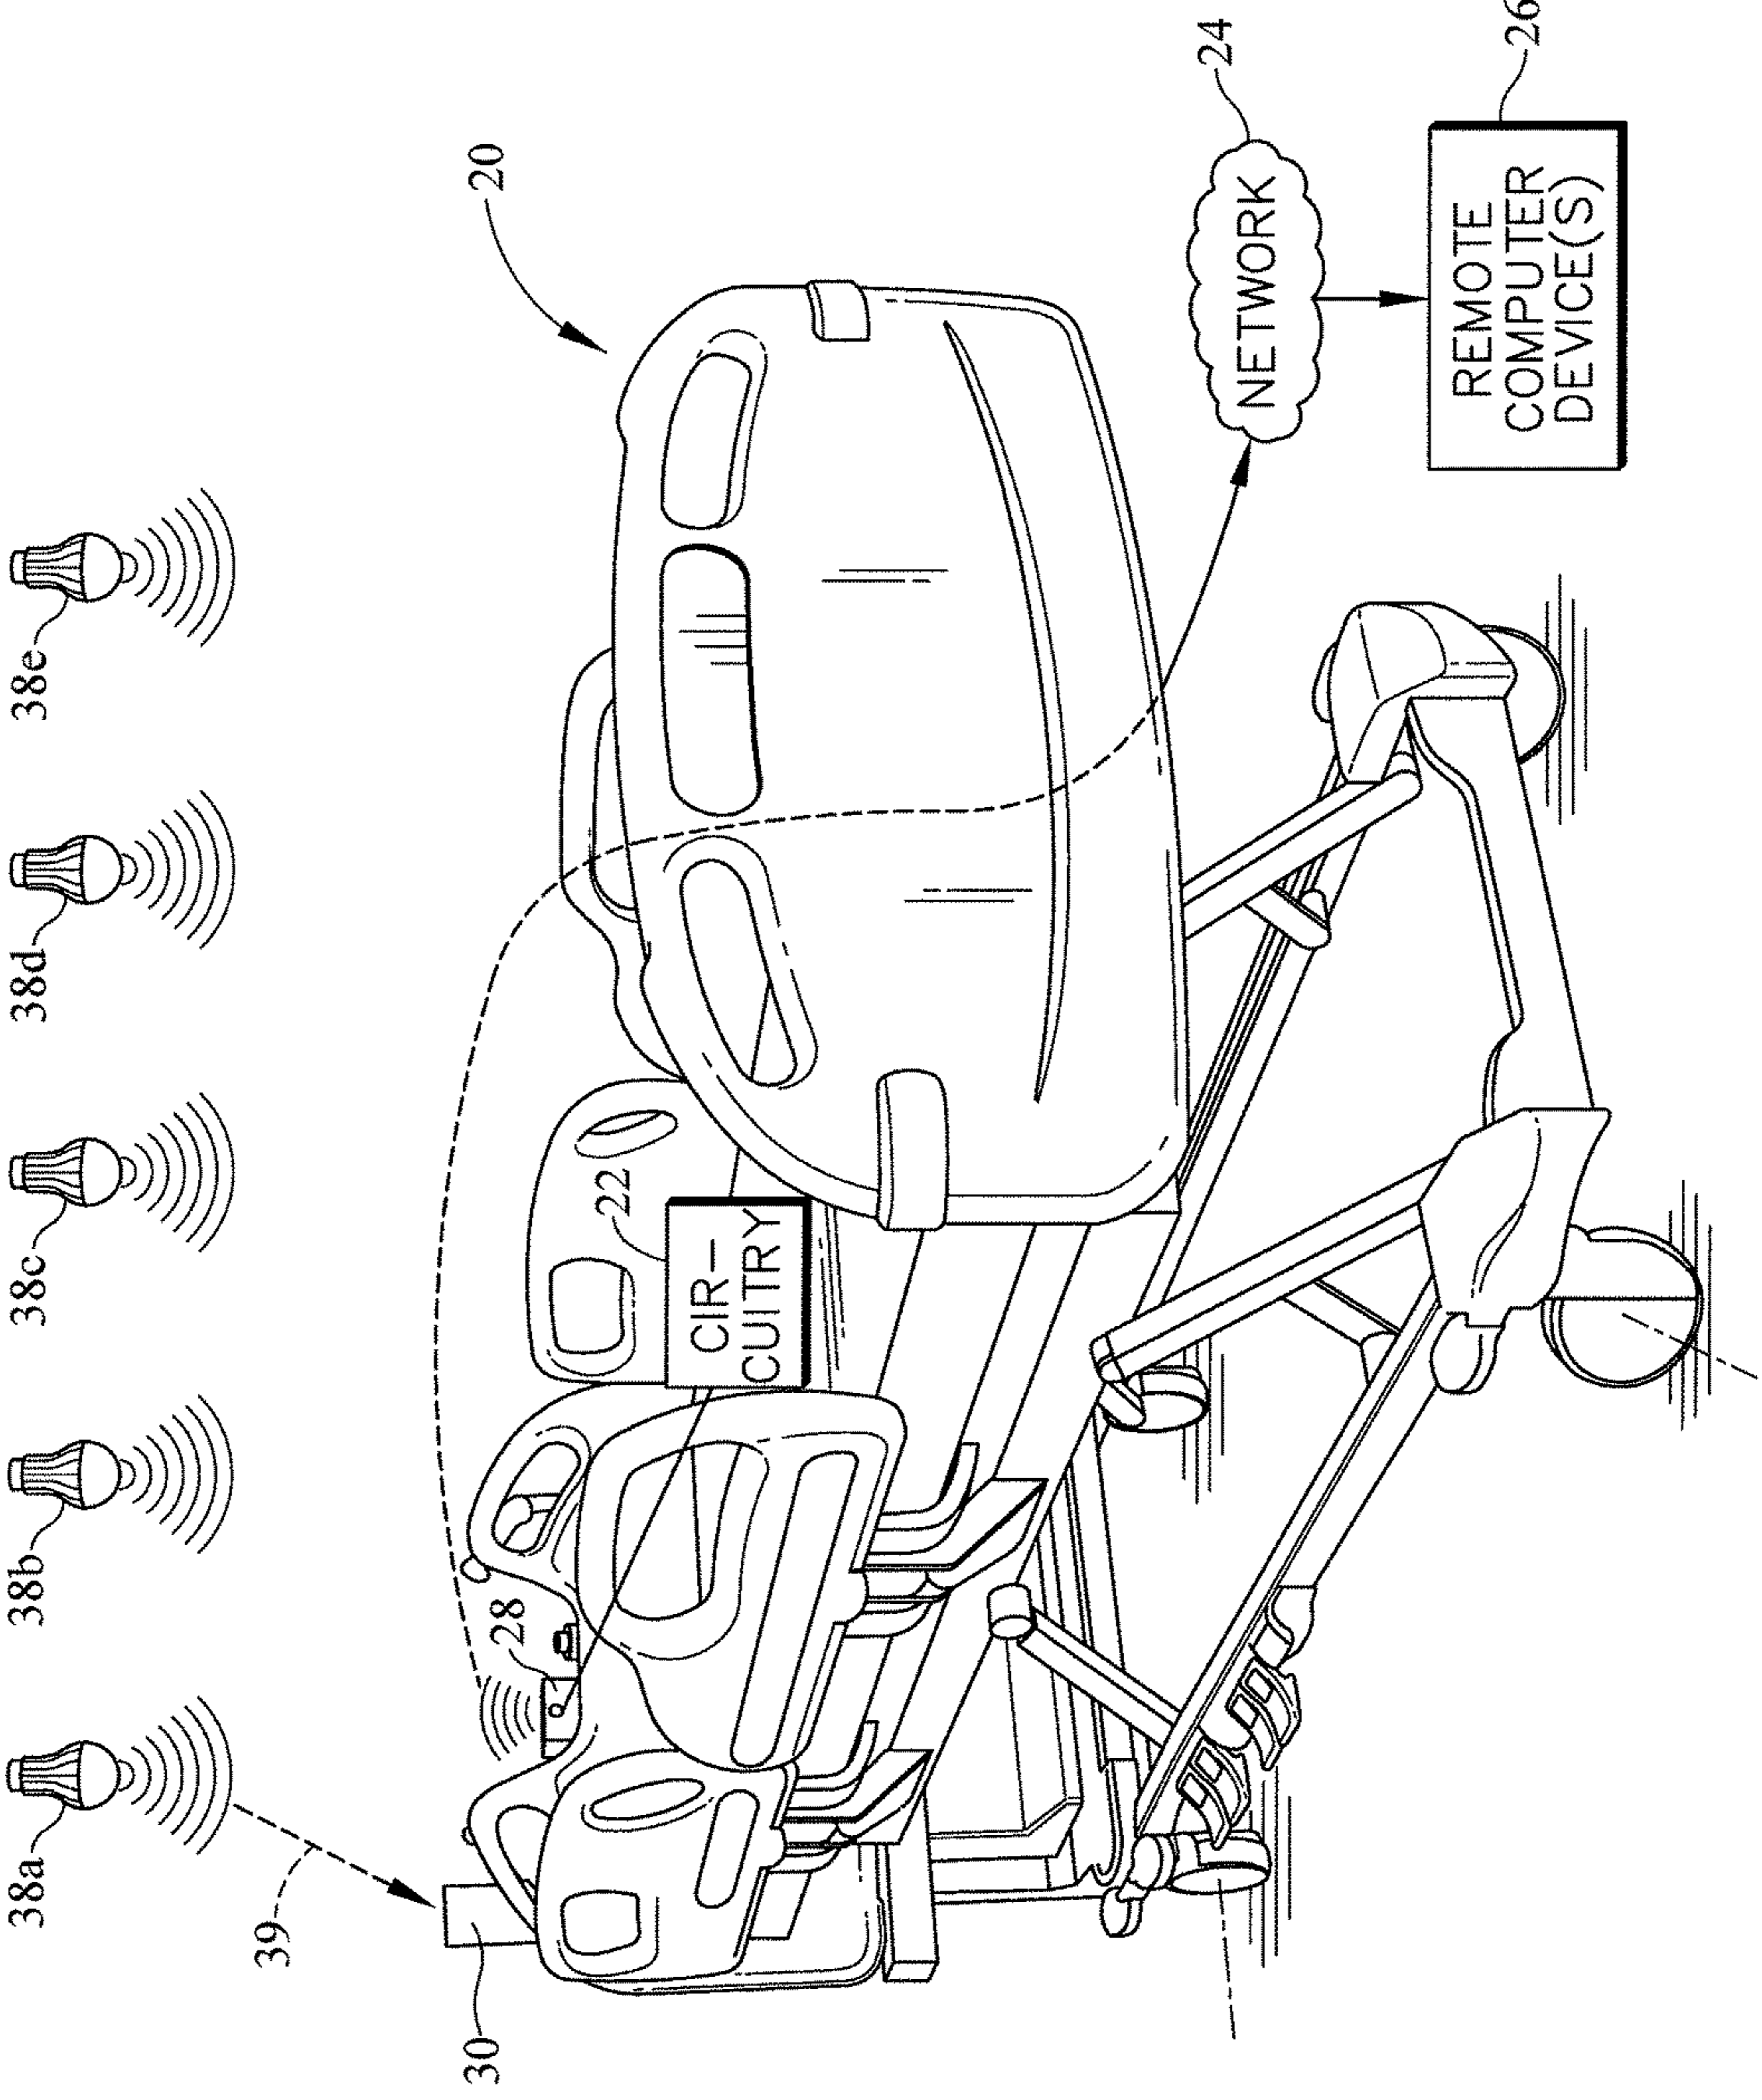


FIG. 2

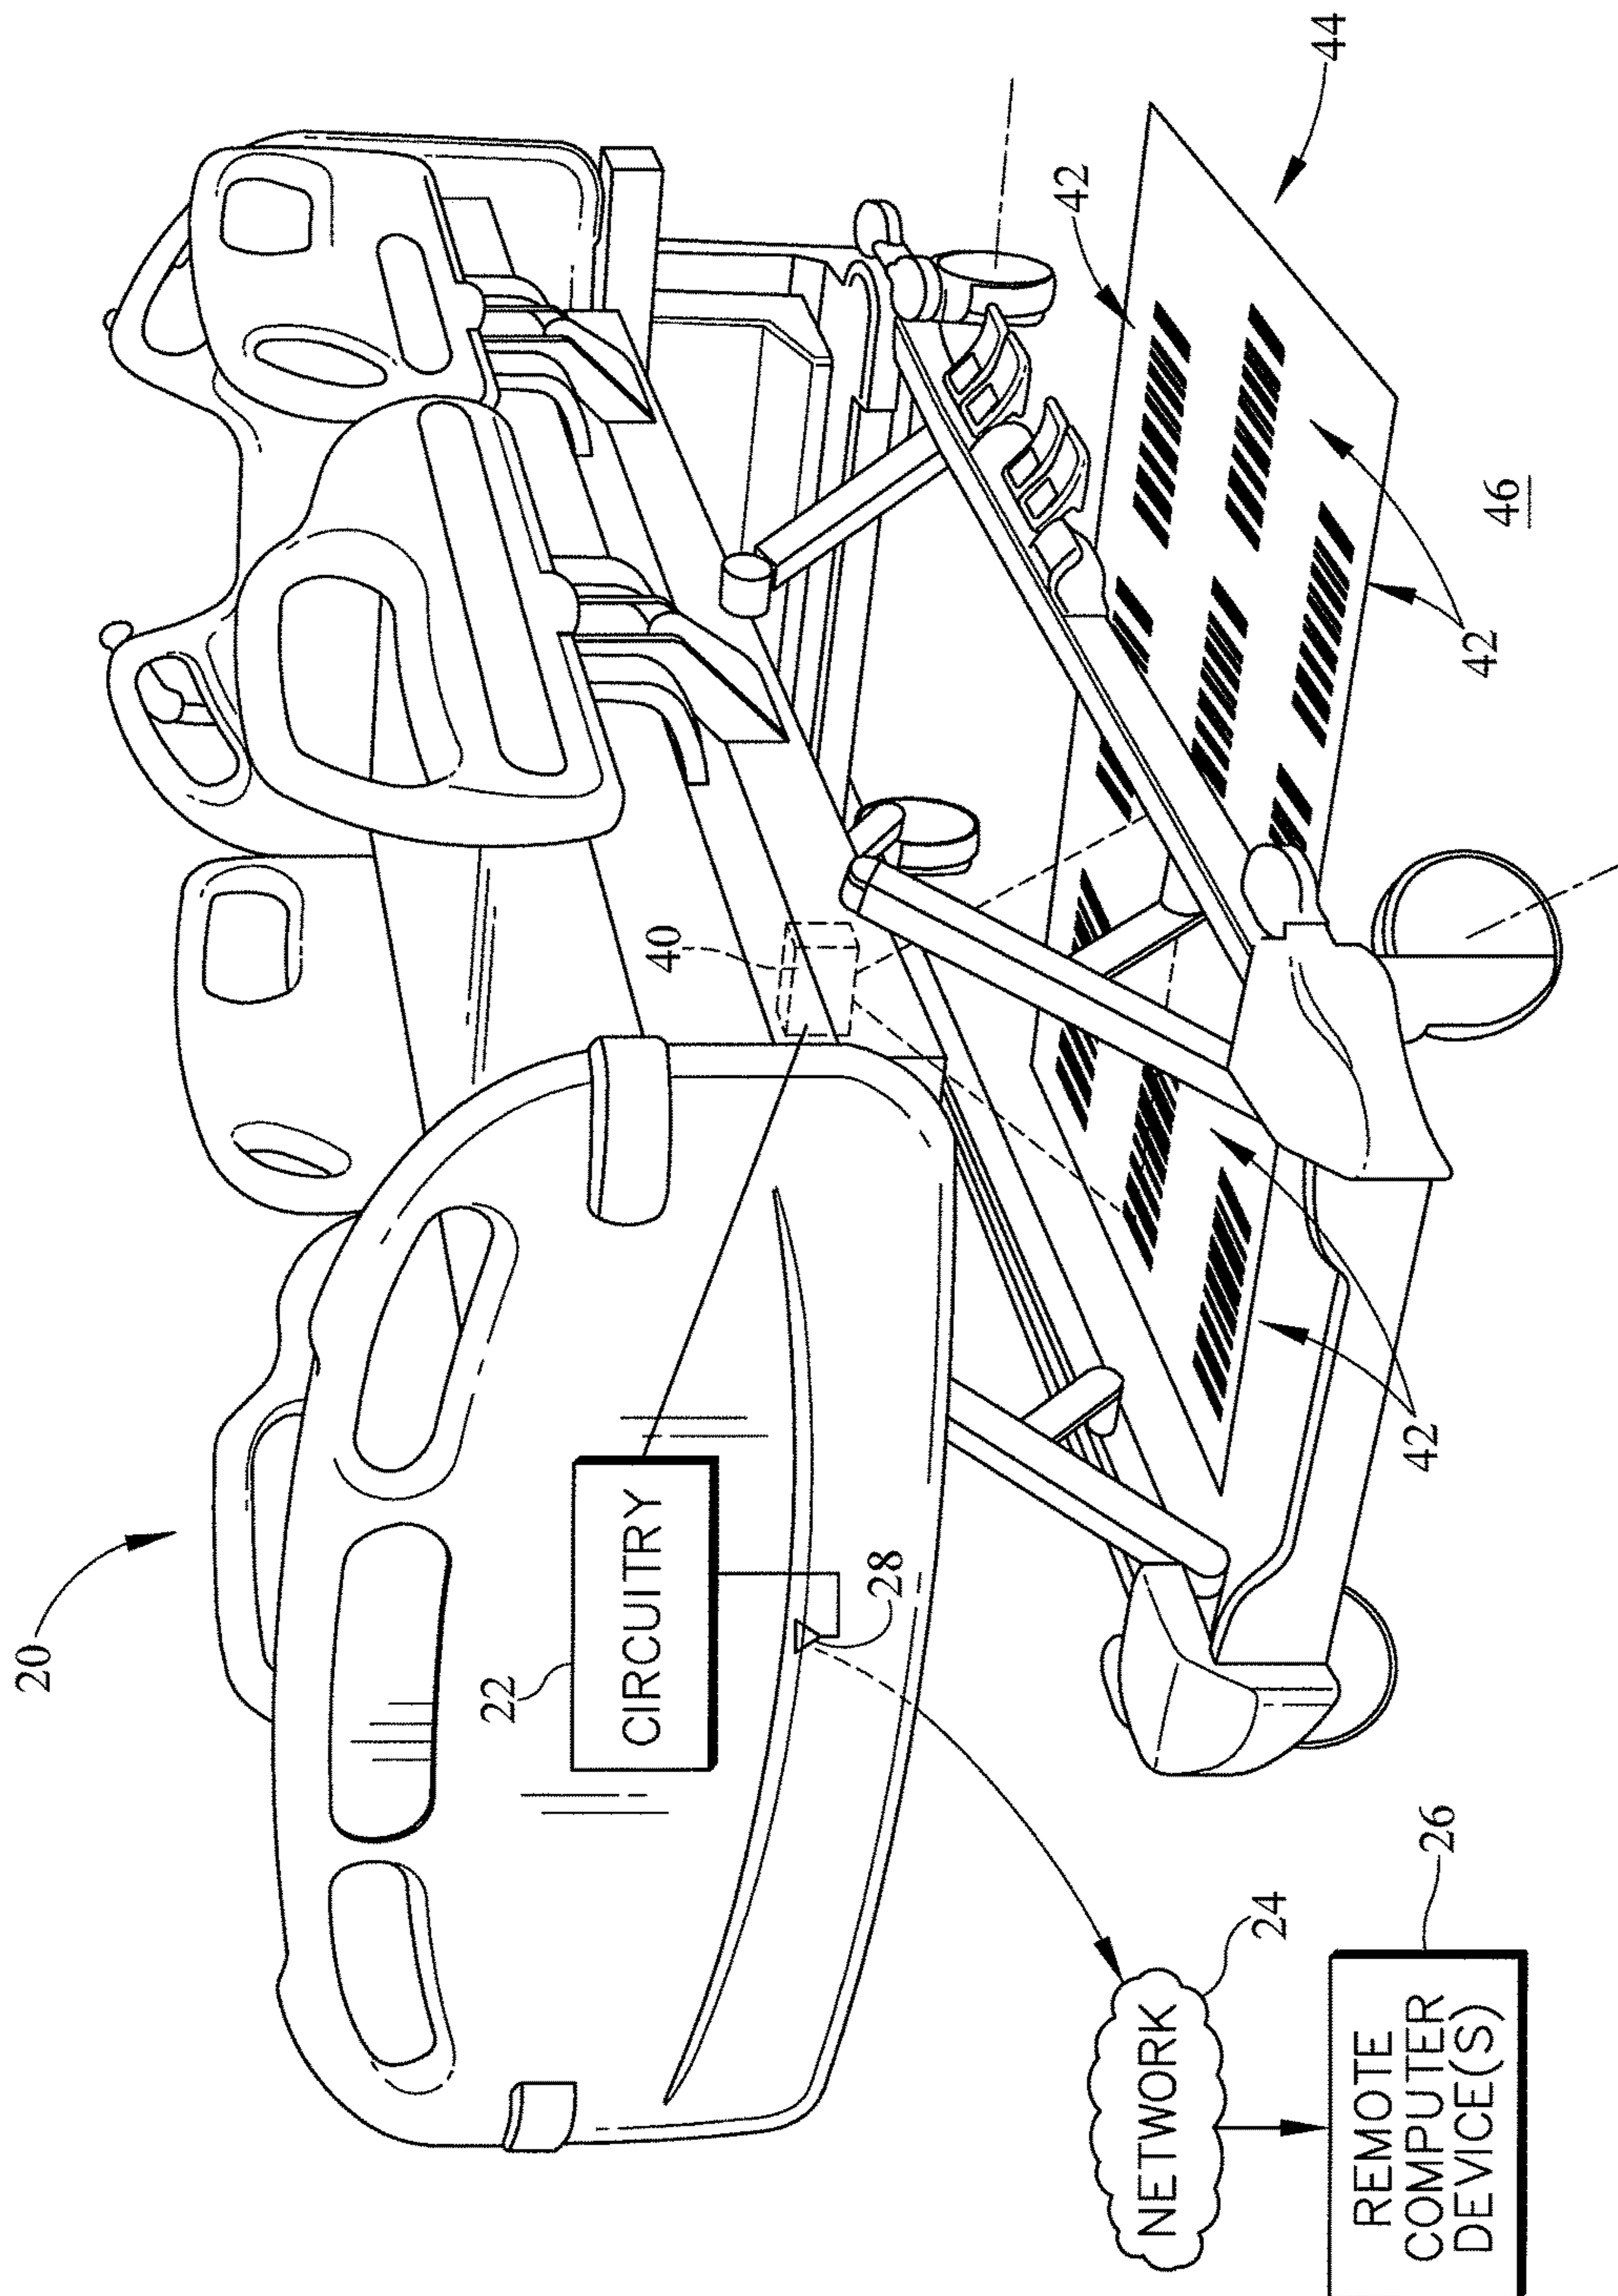


FIG. 3

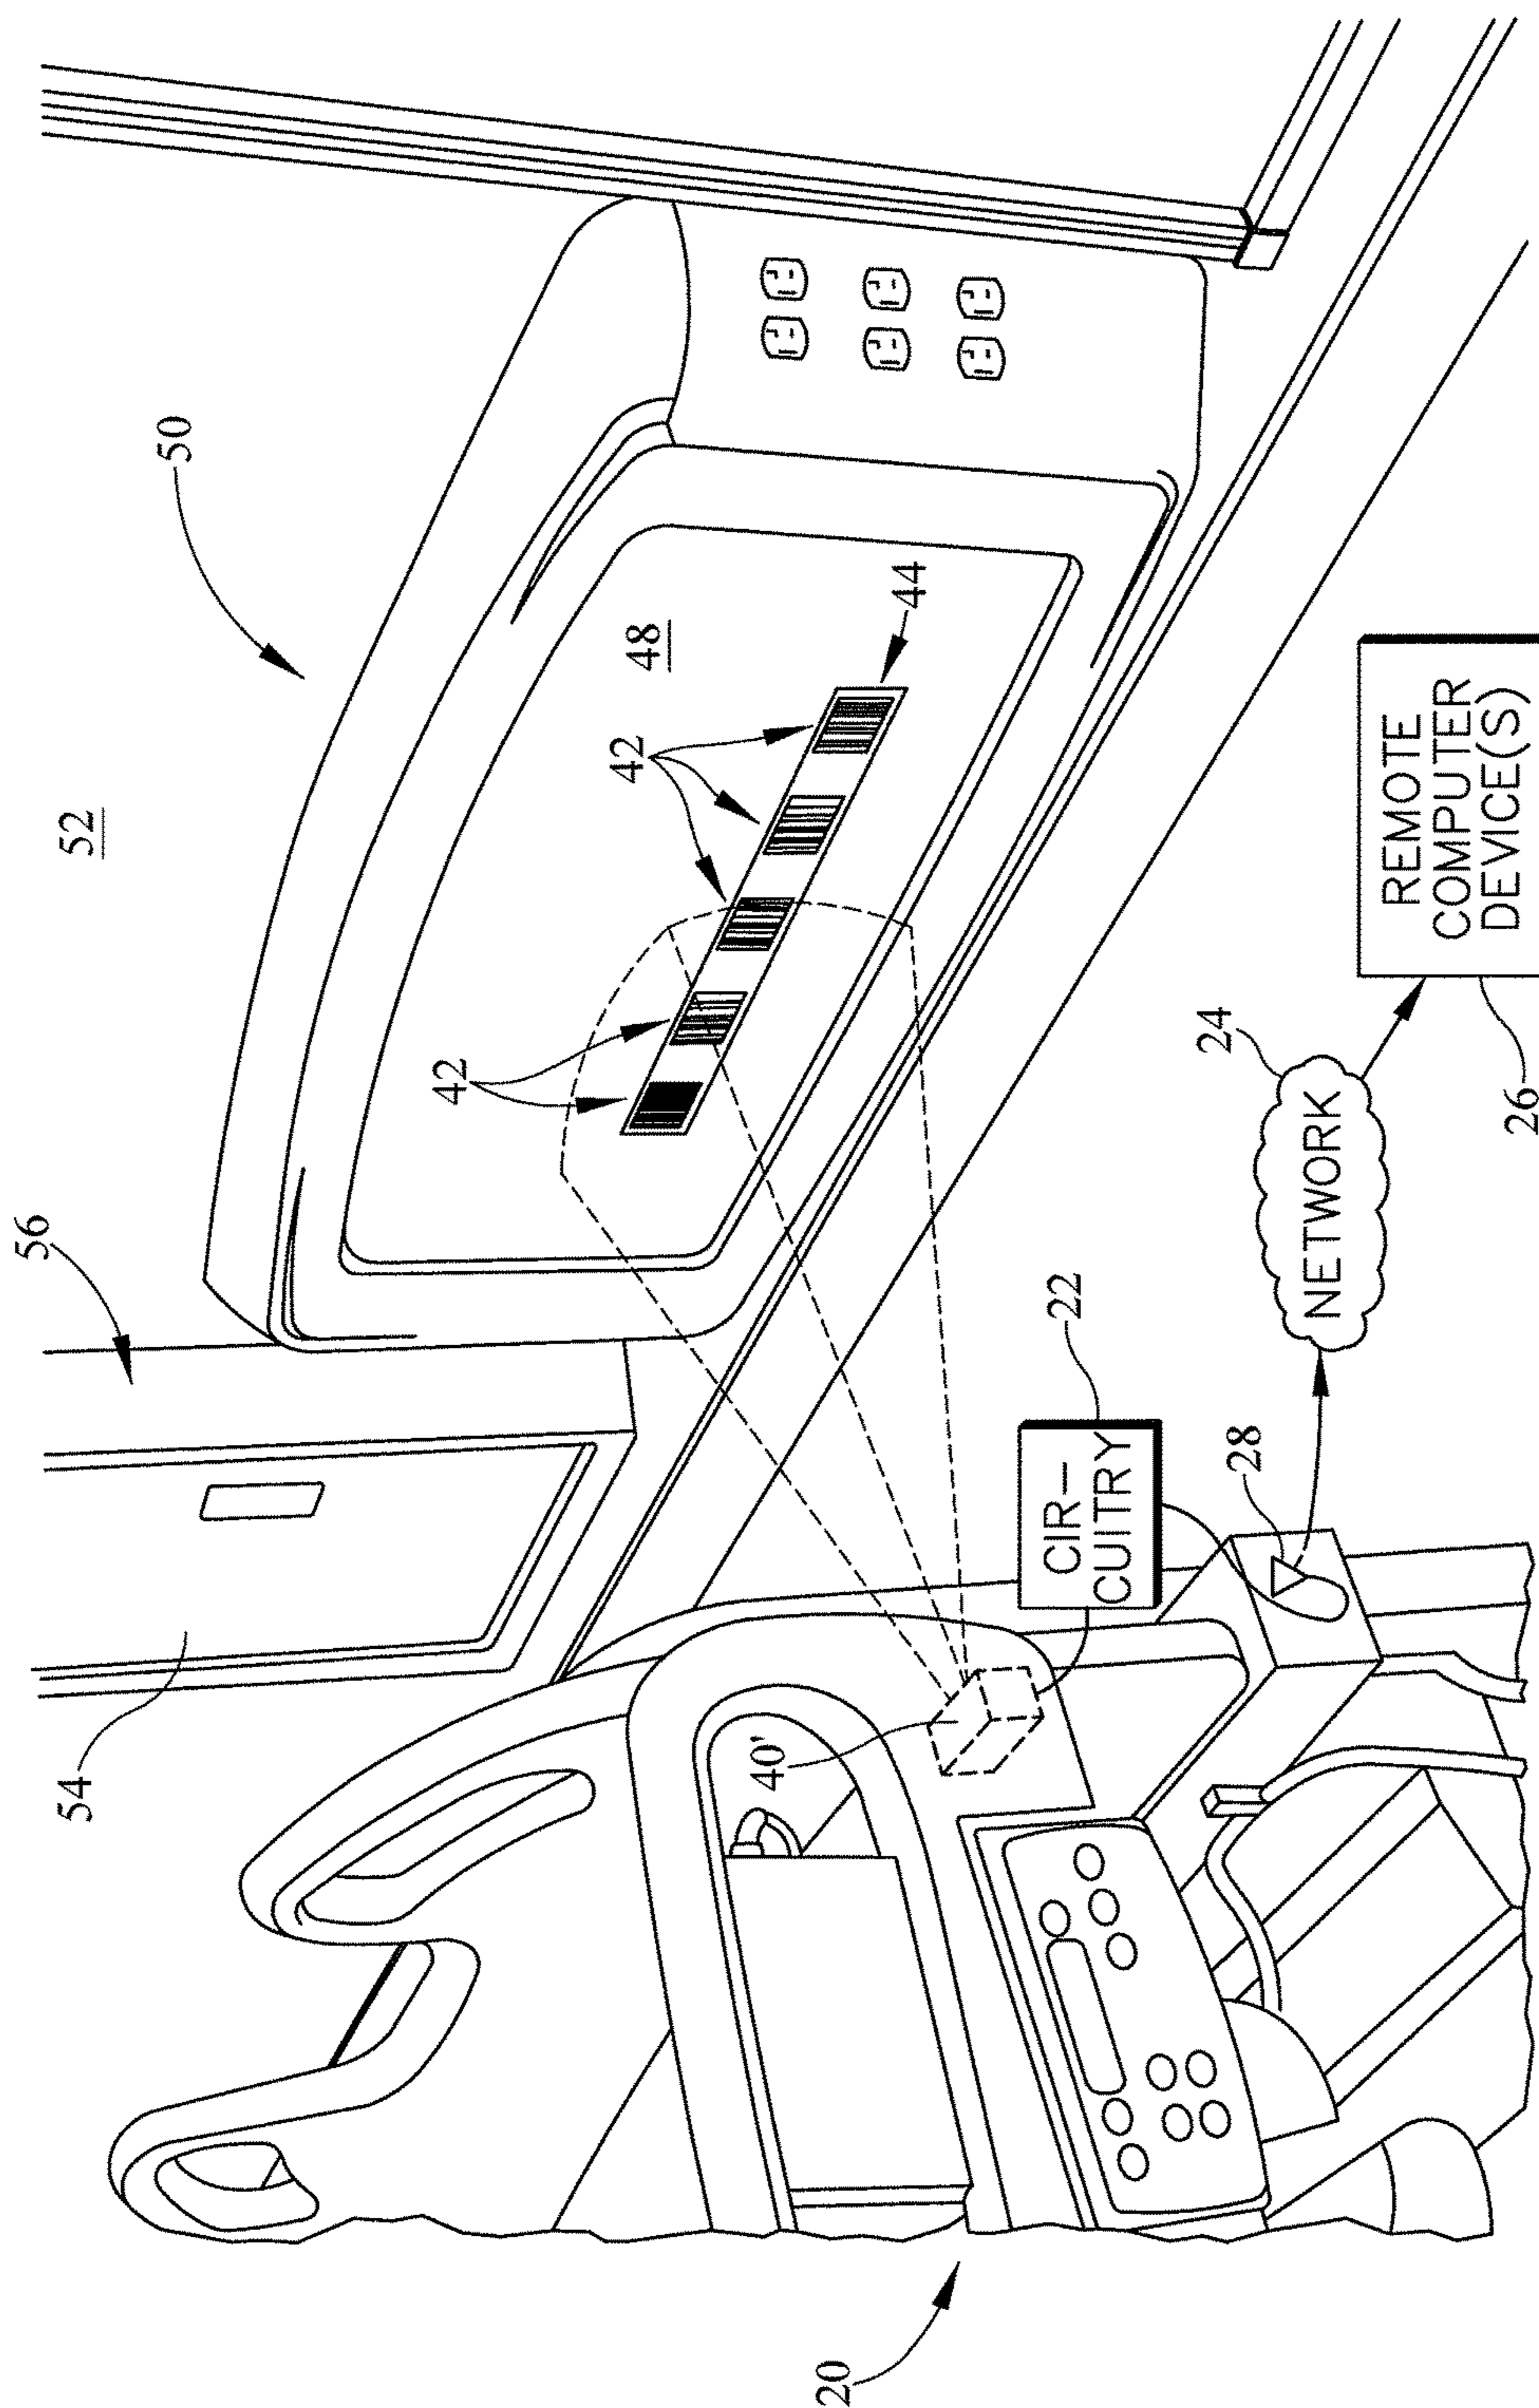


FIG. 4

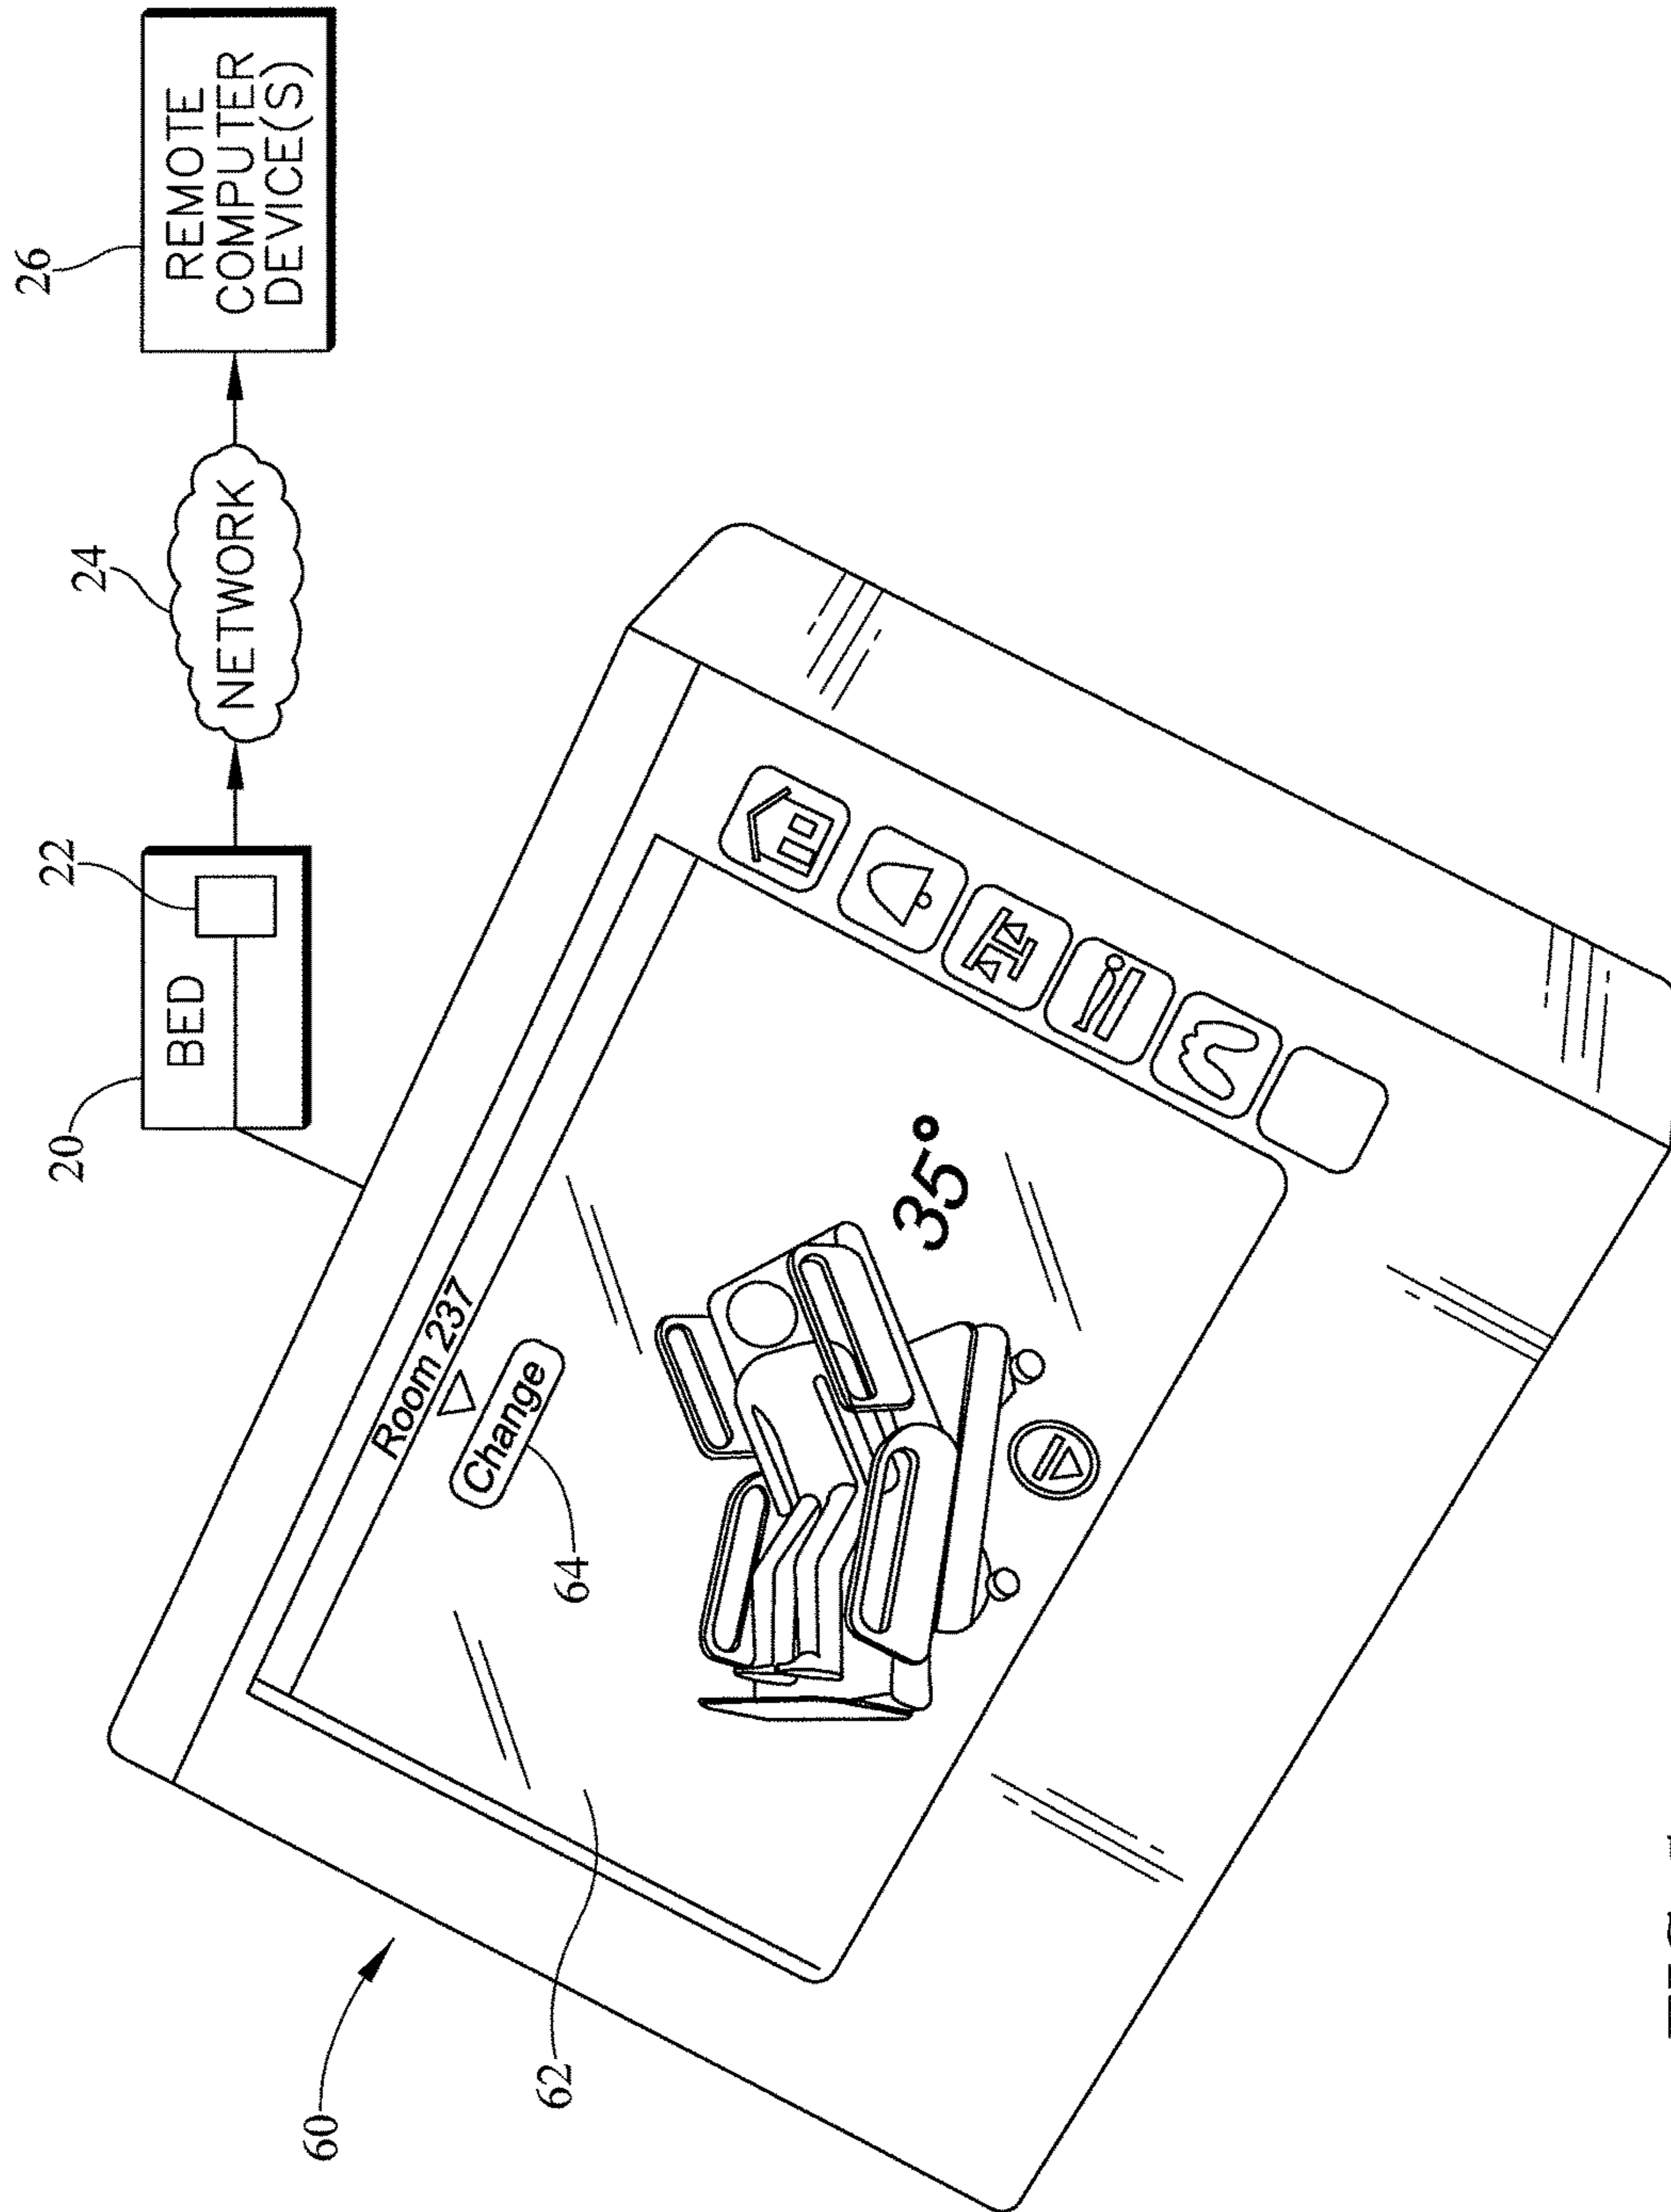


FIG. 5

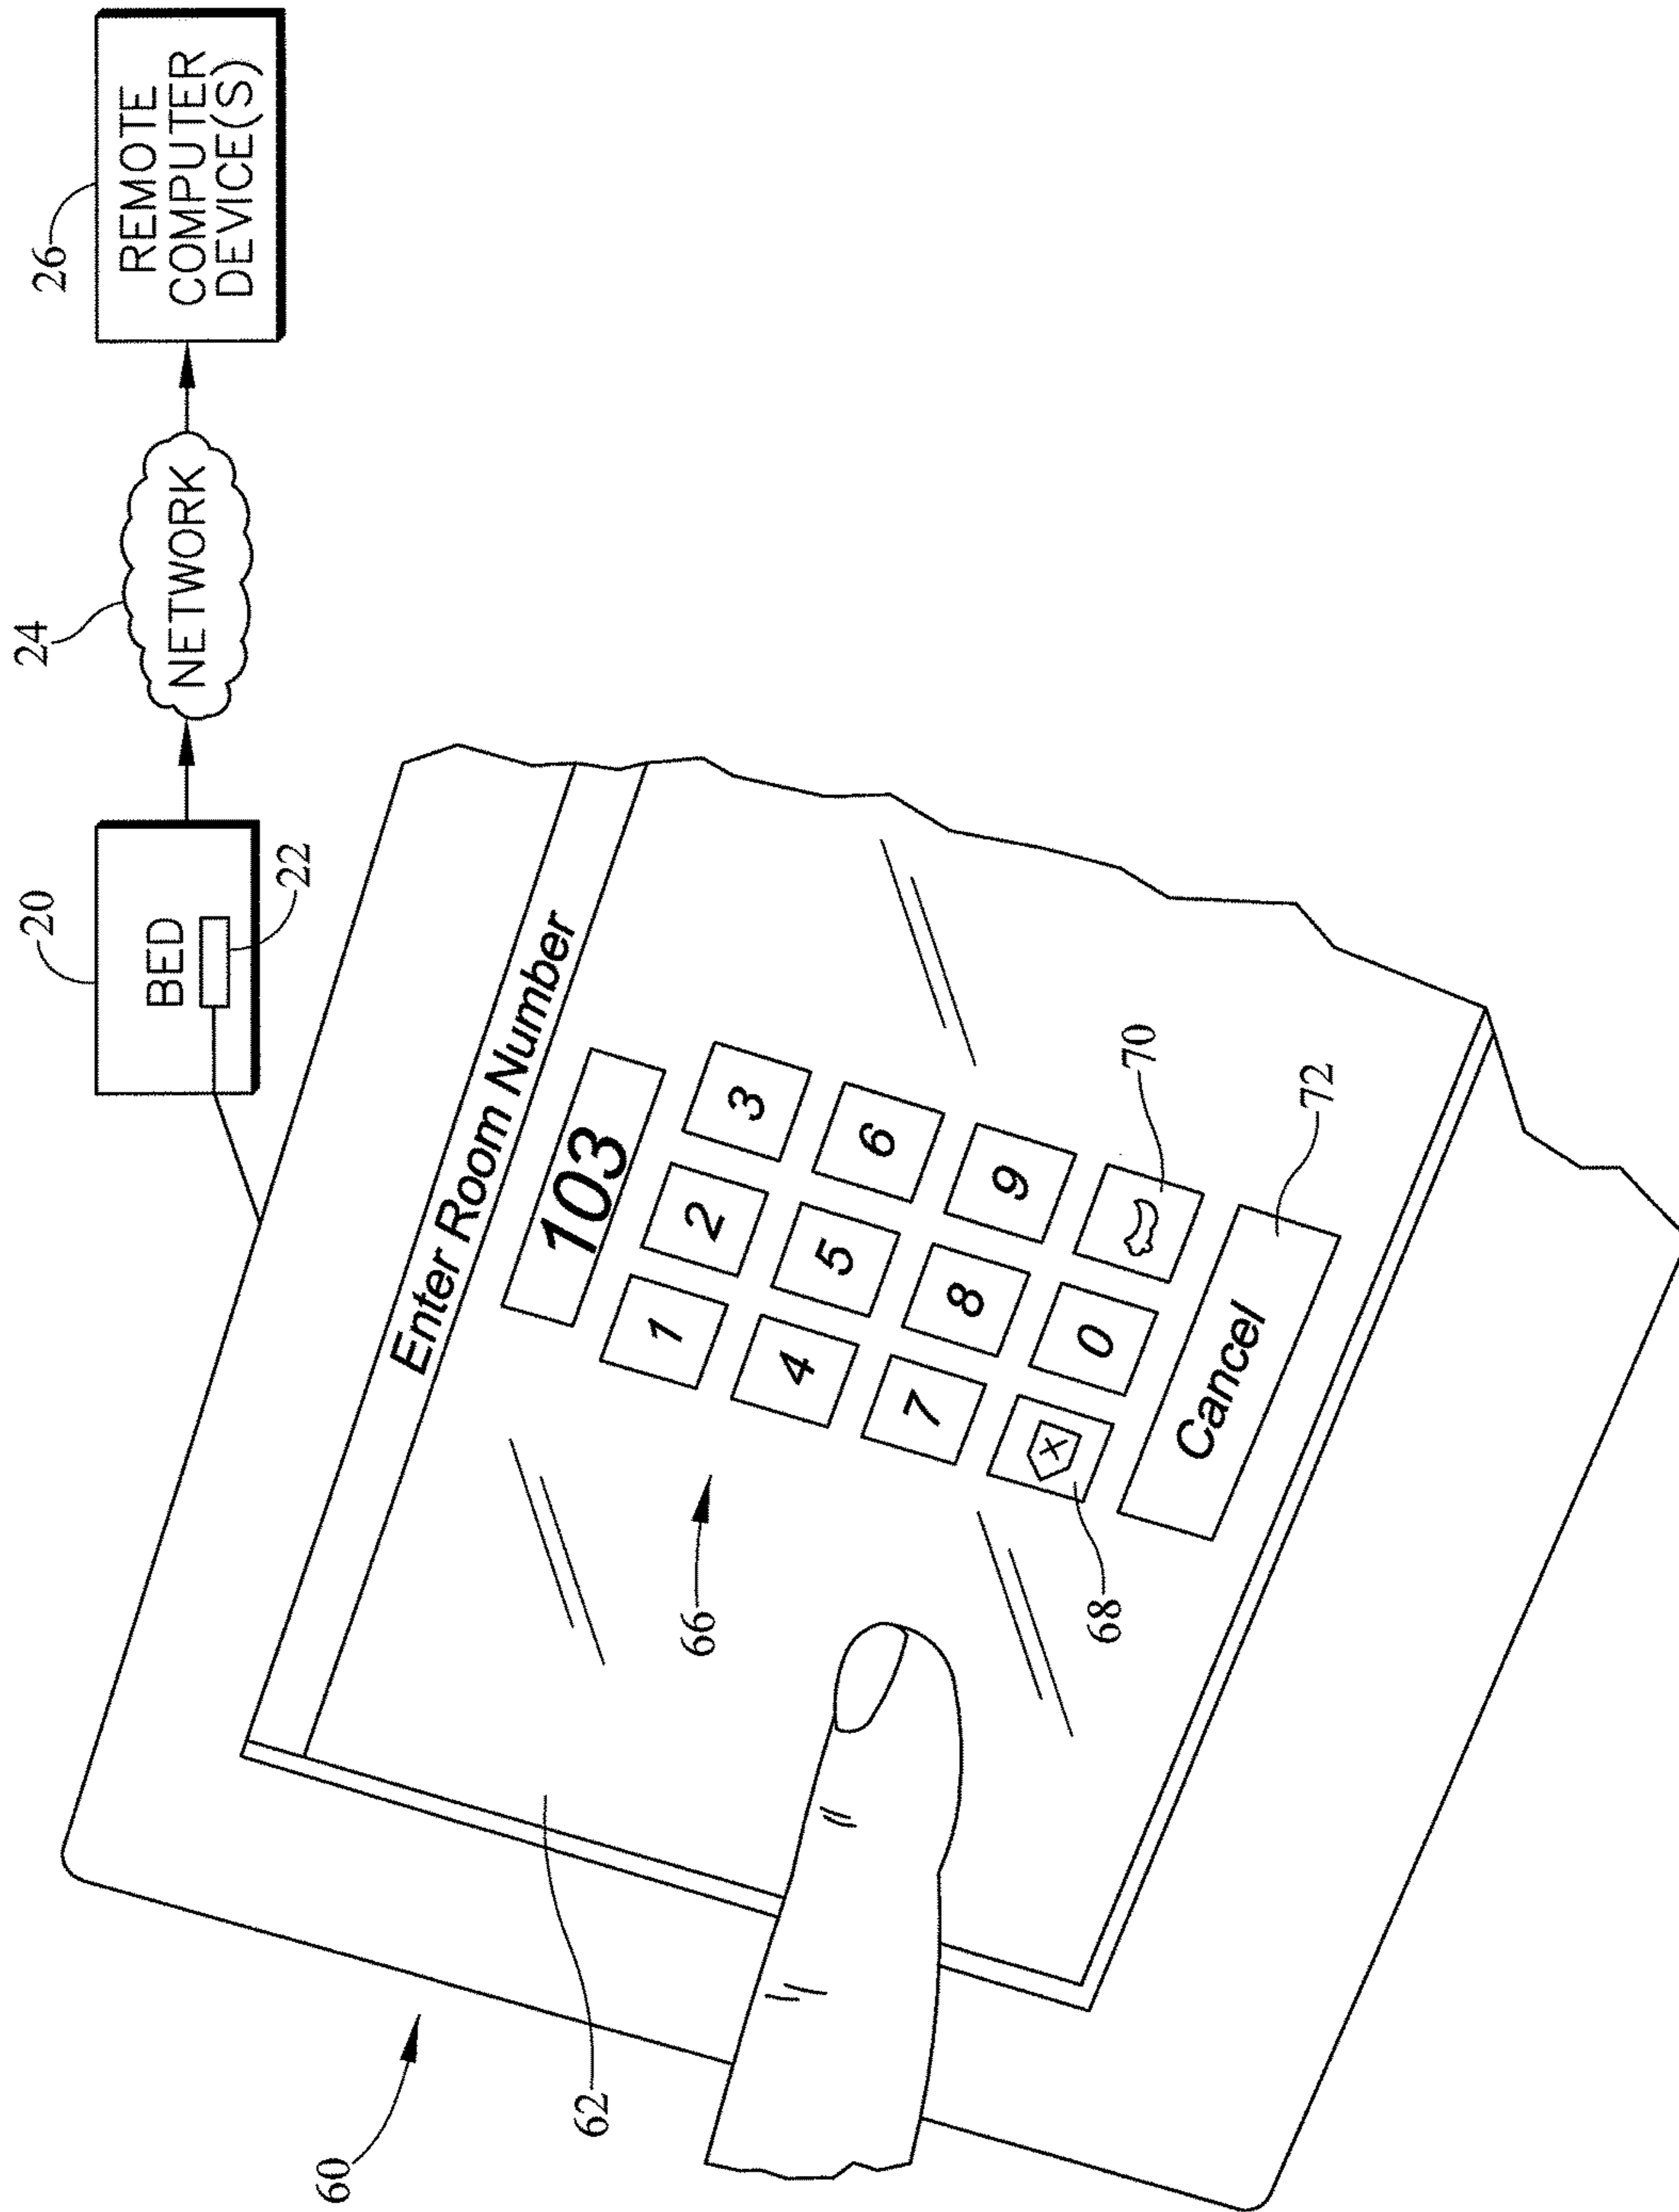


FIG. 6

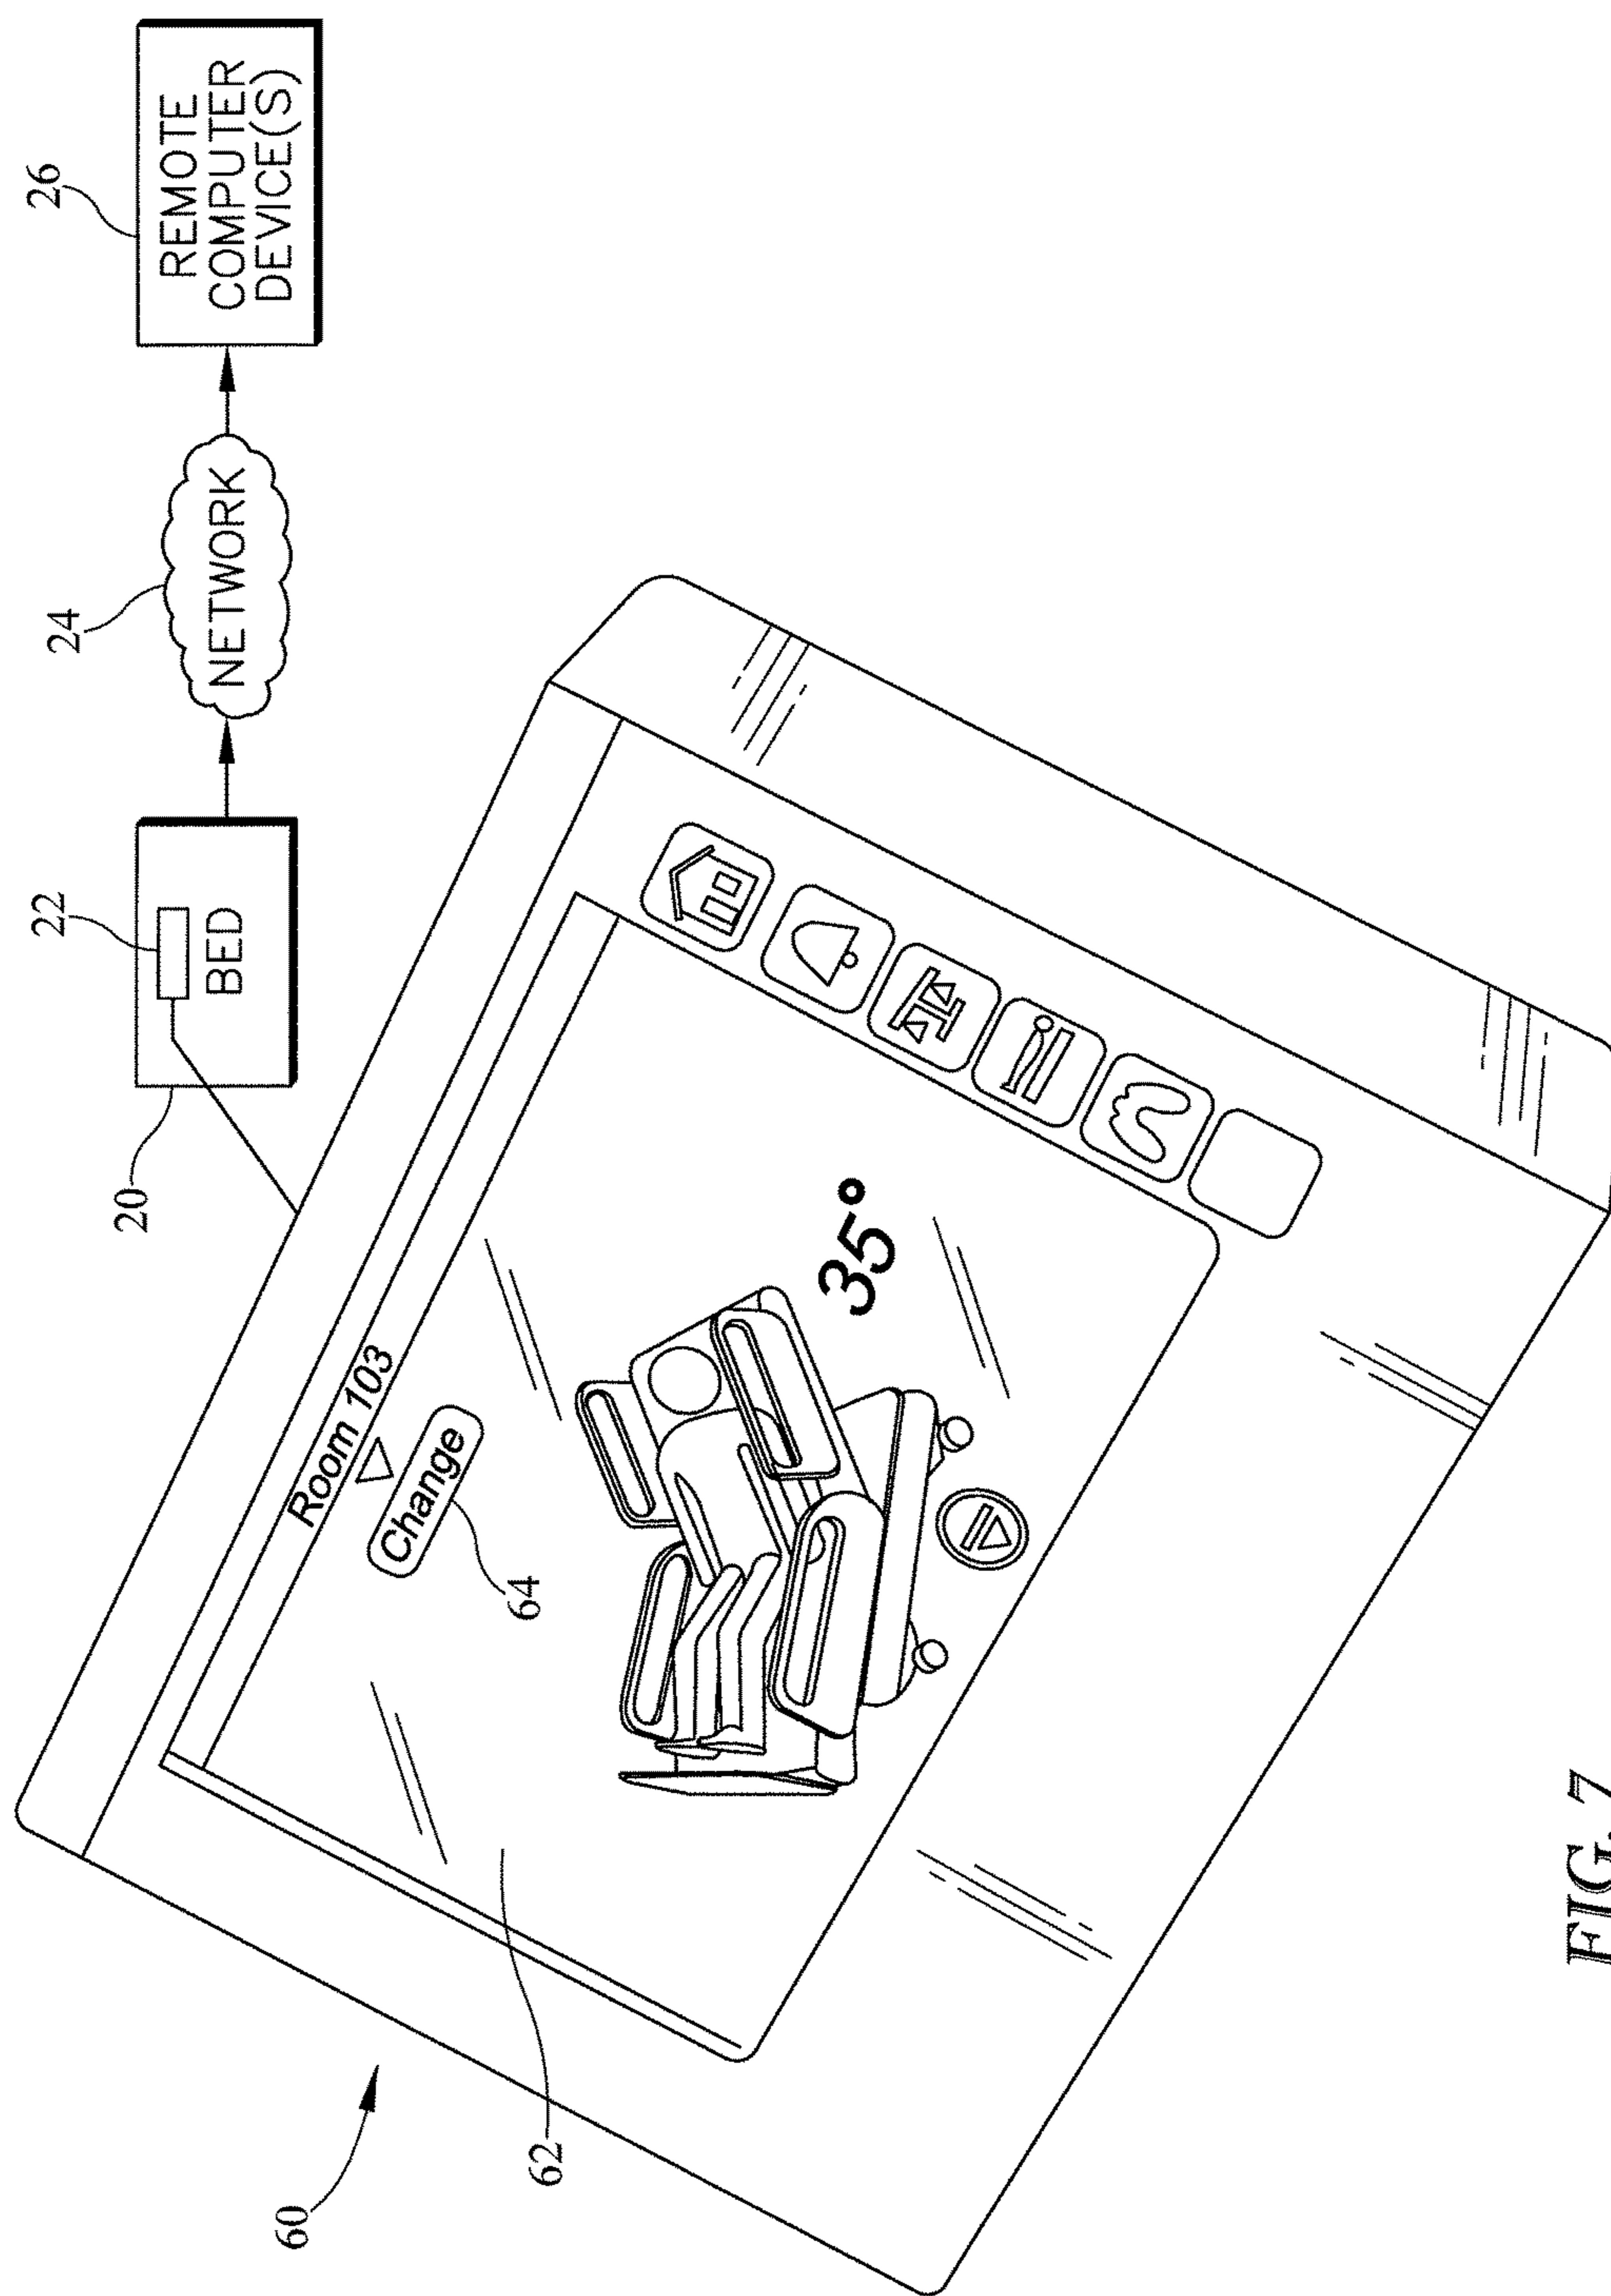


FIG. 7

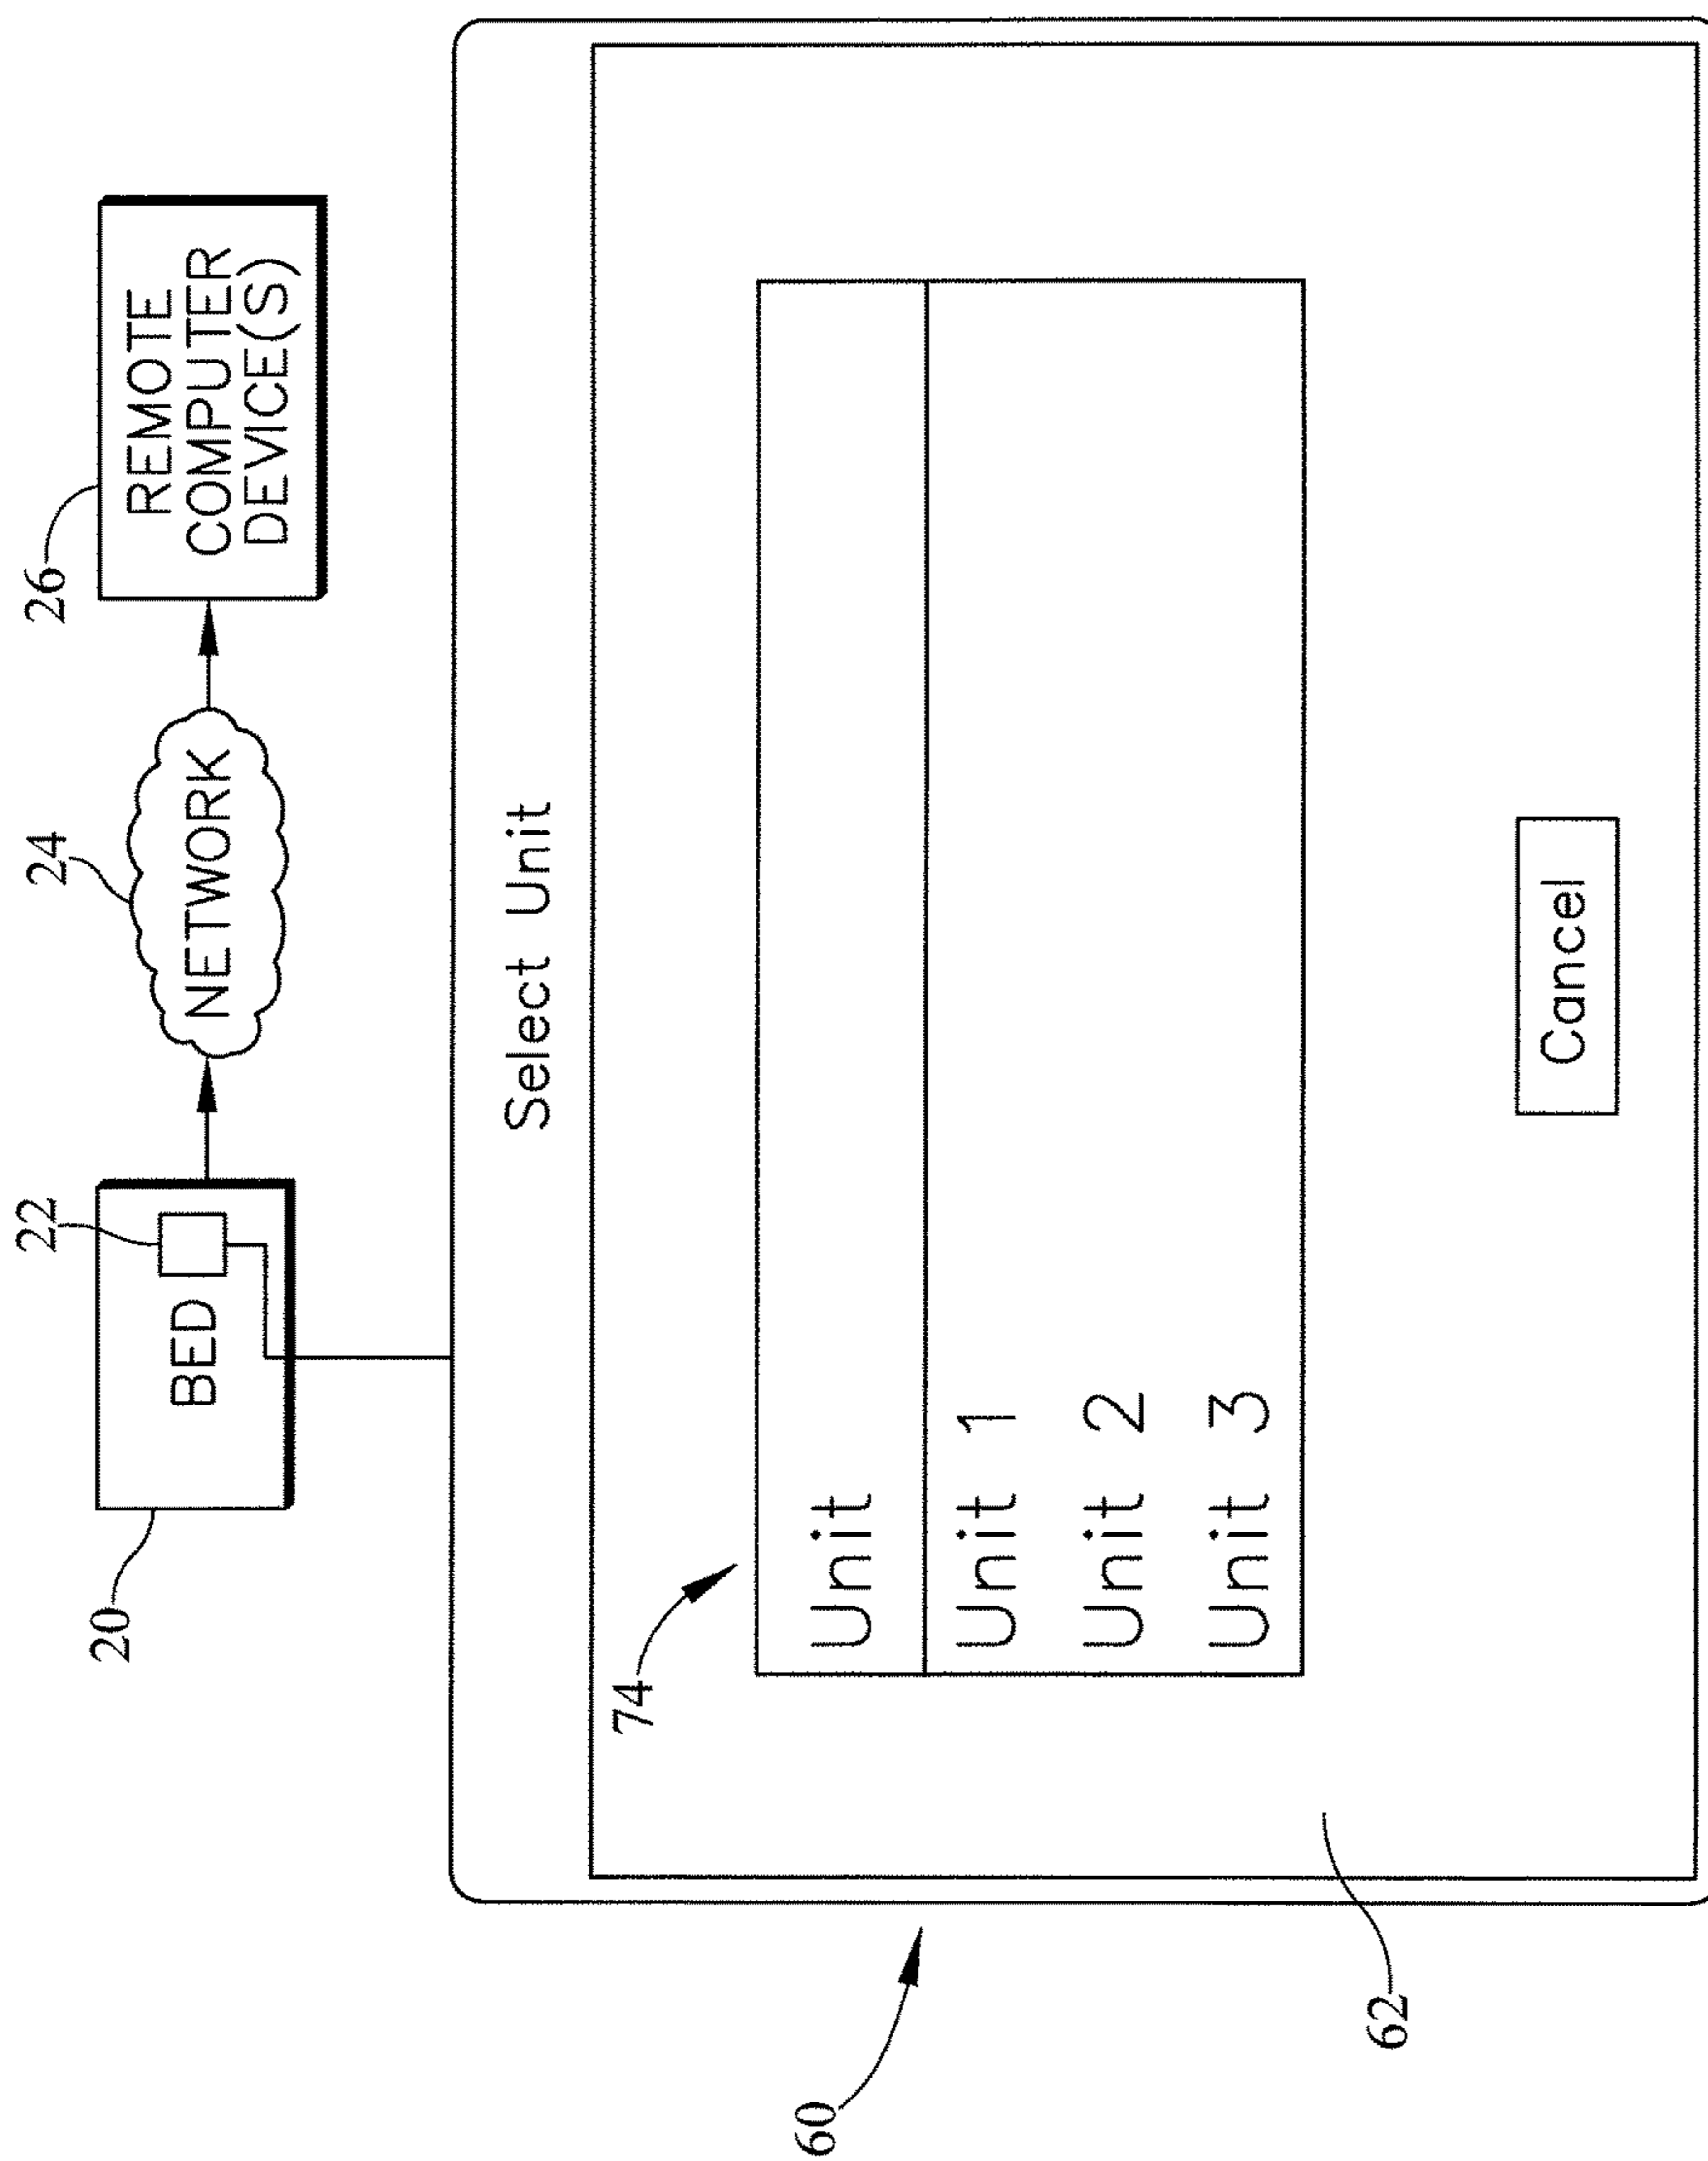


FIG. 8

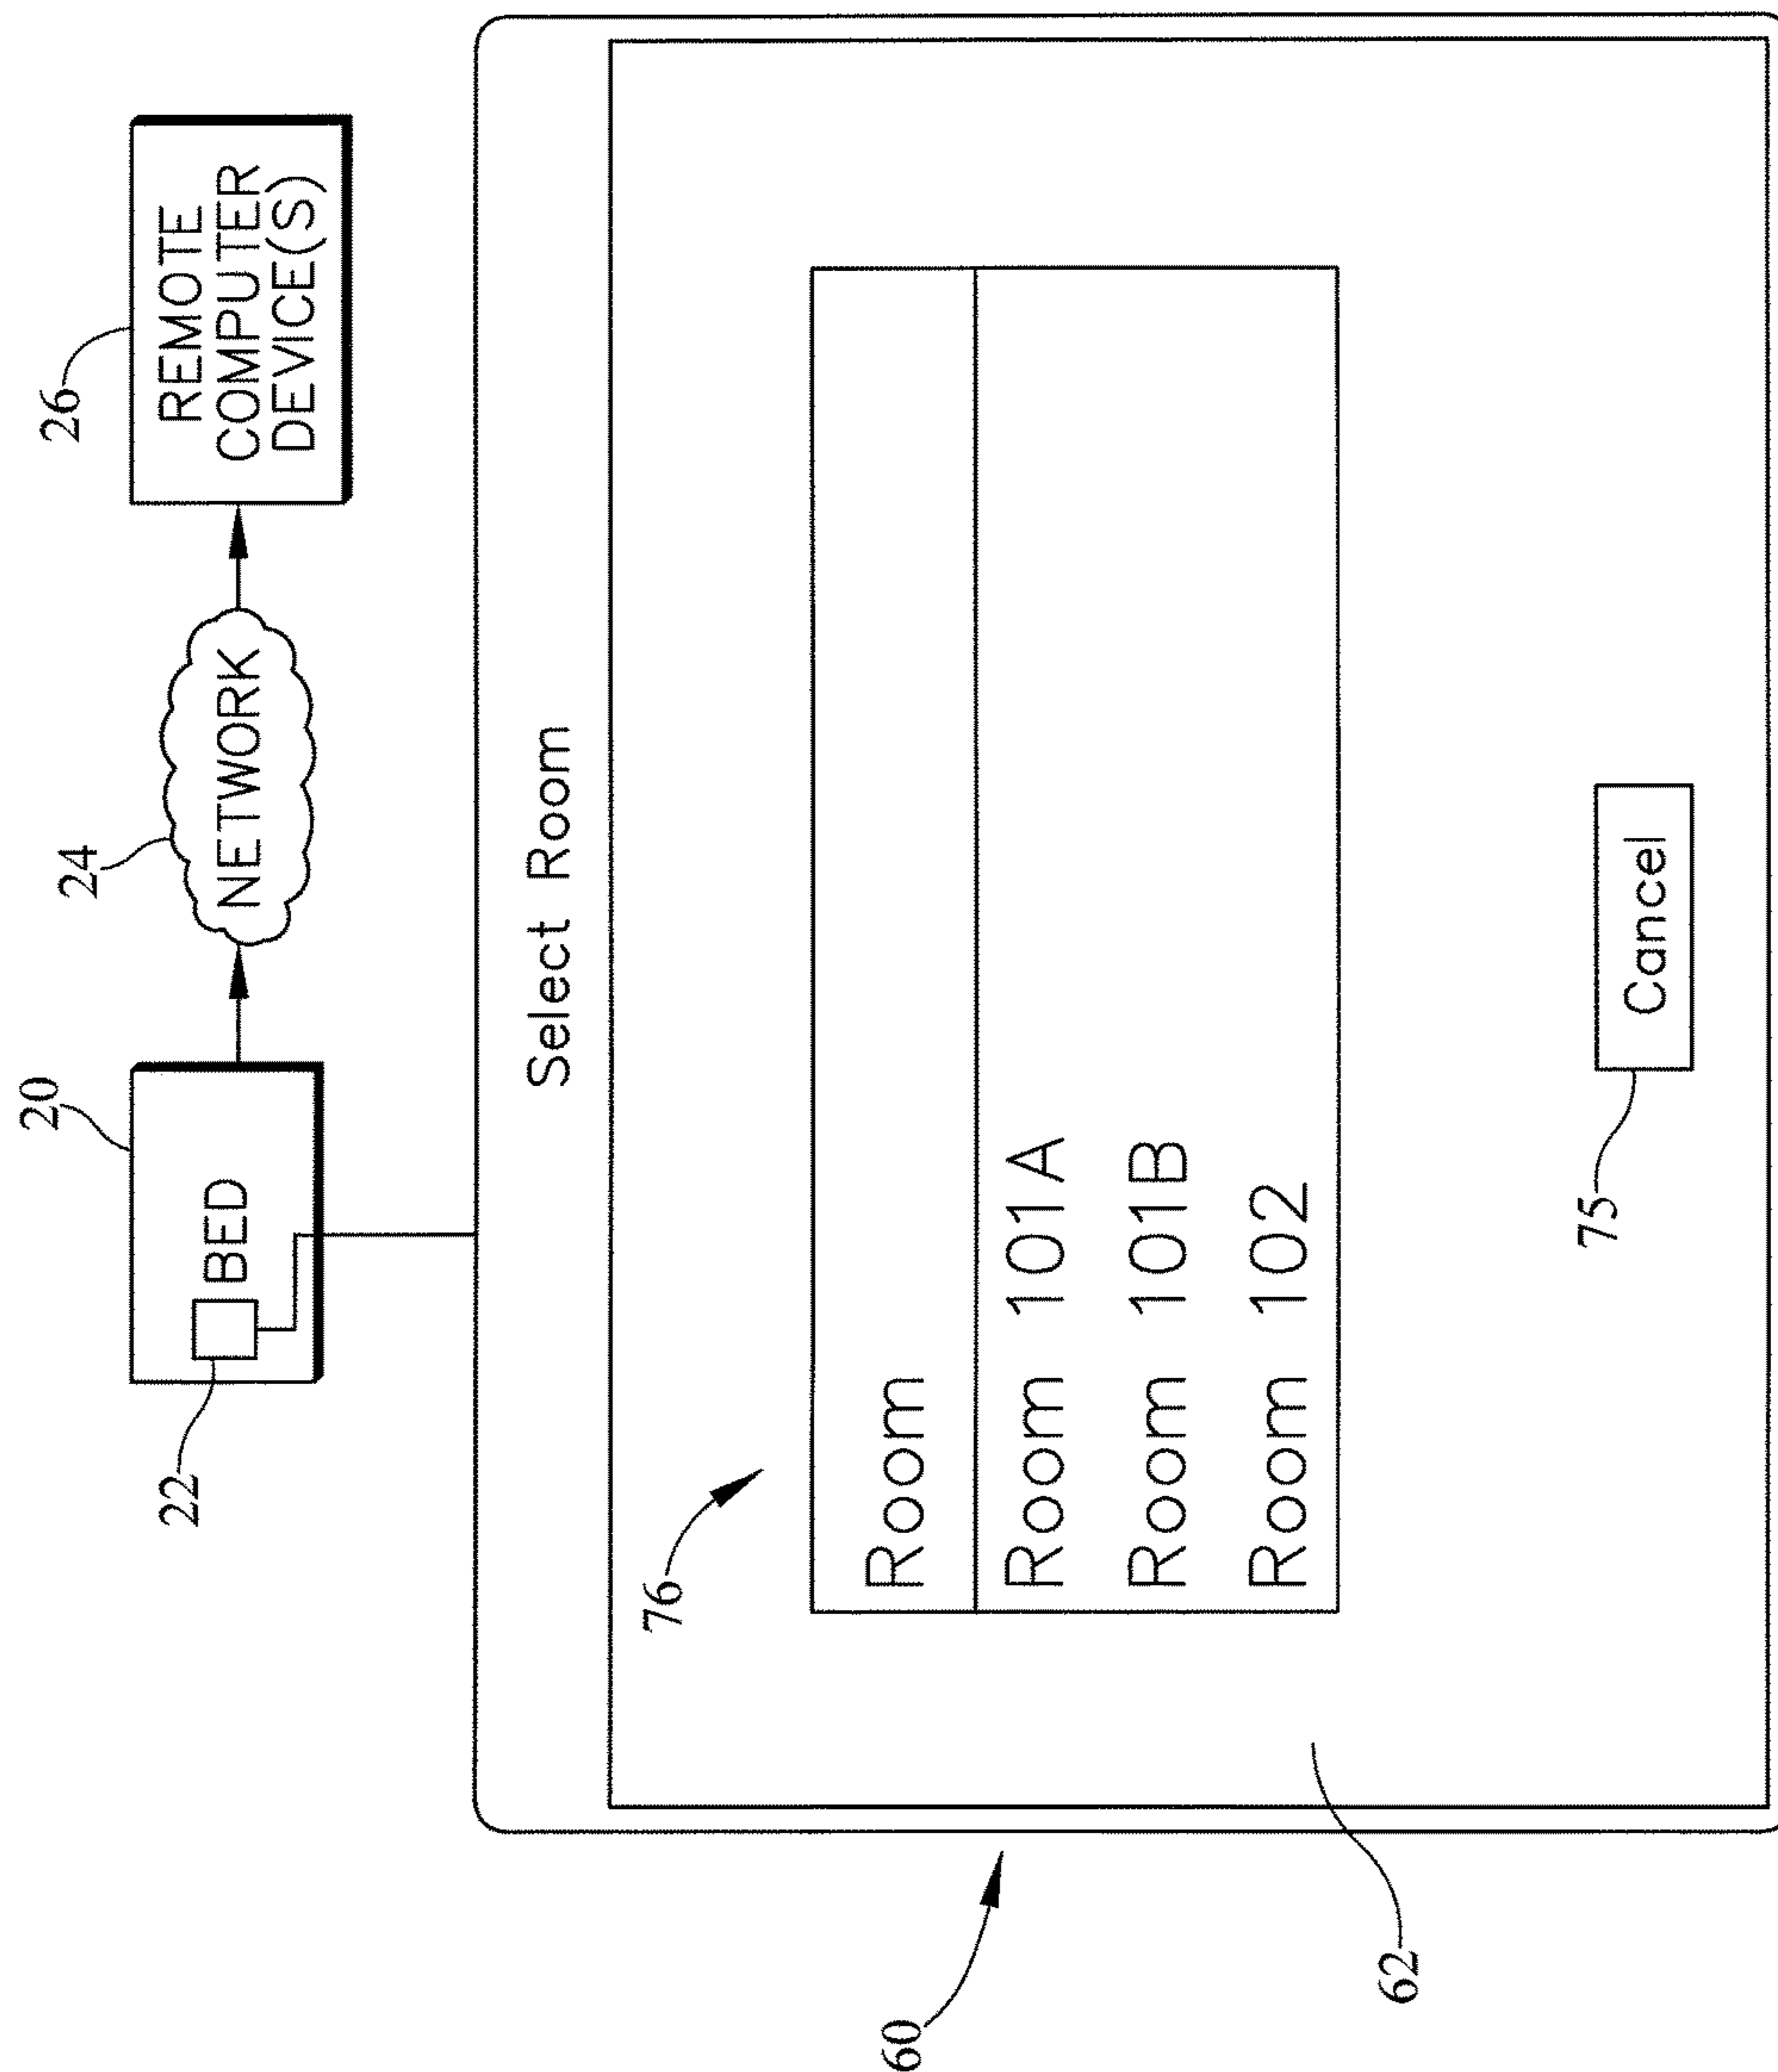


FIG. 9

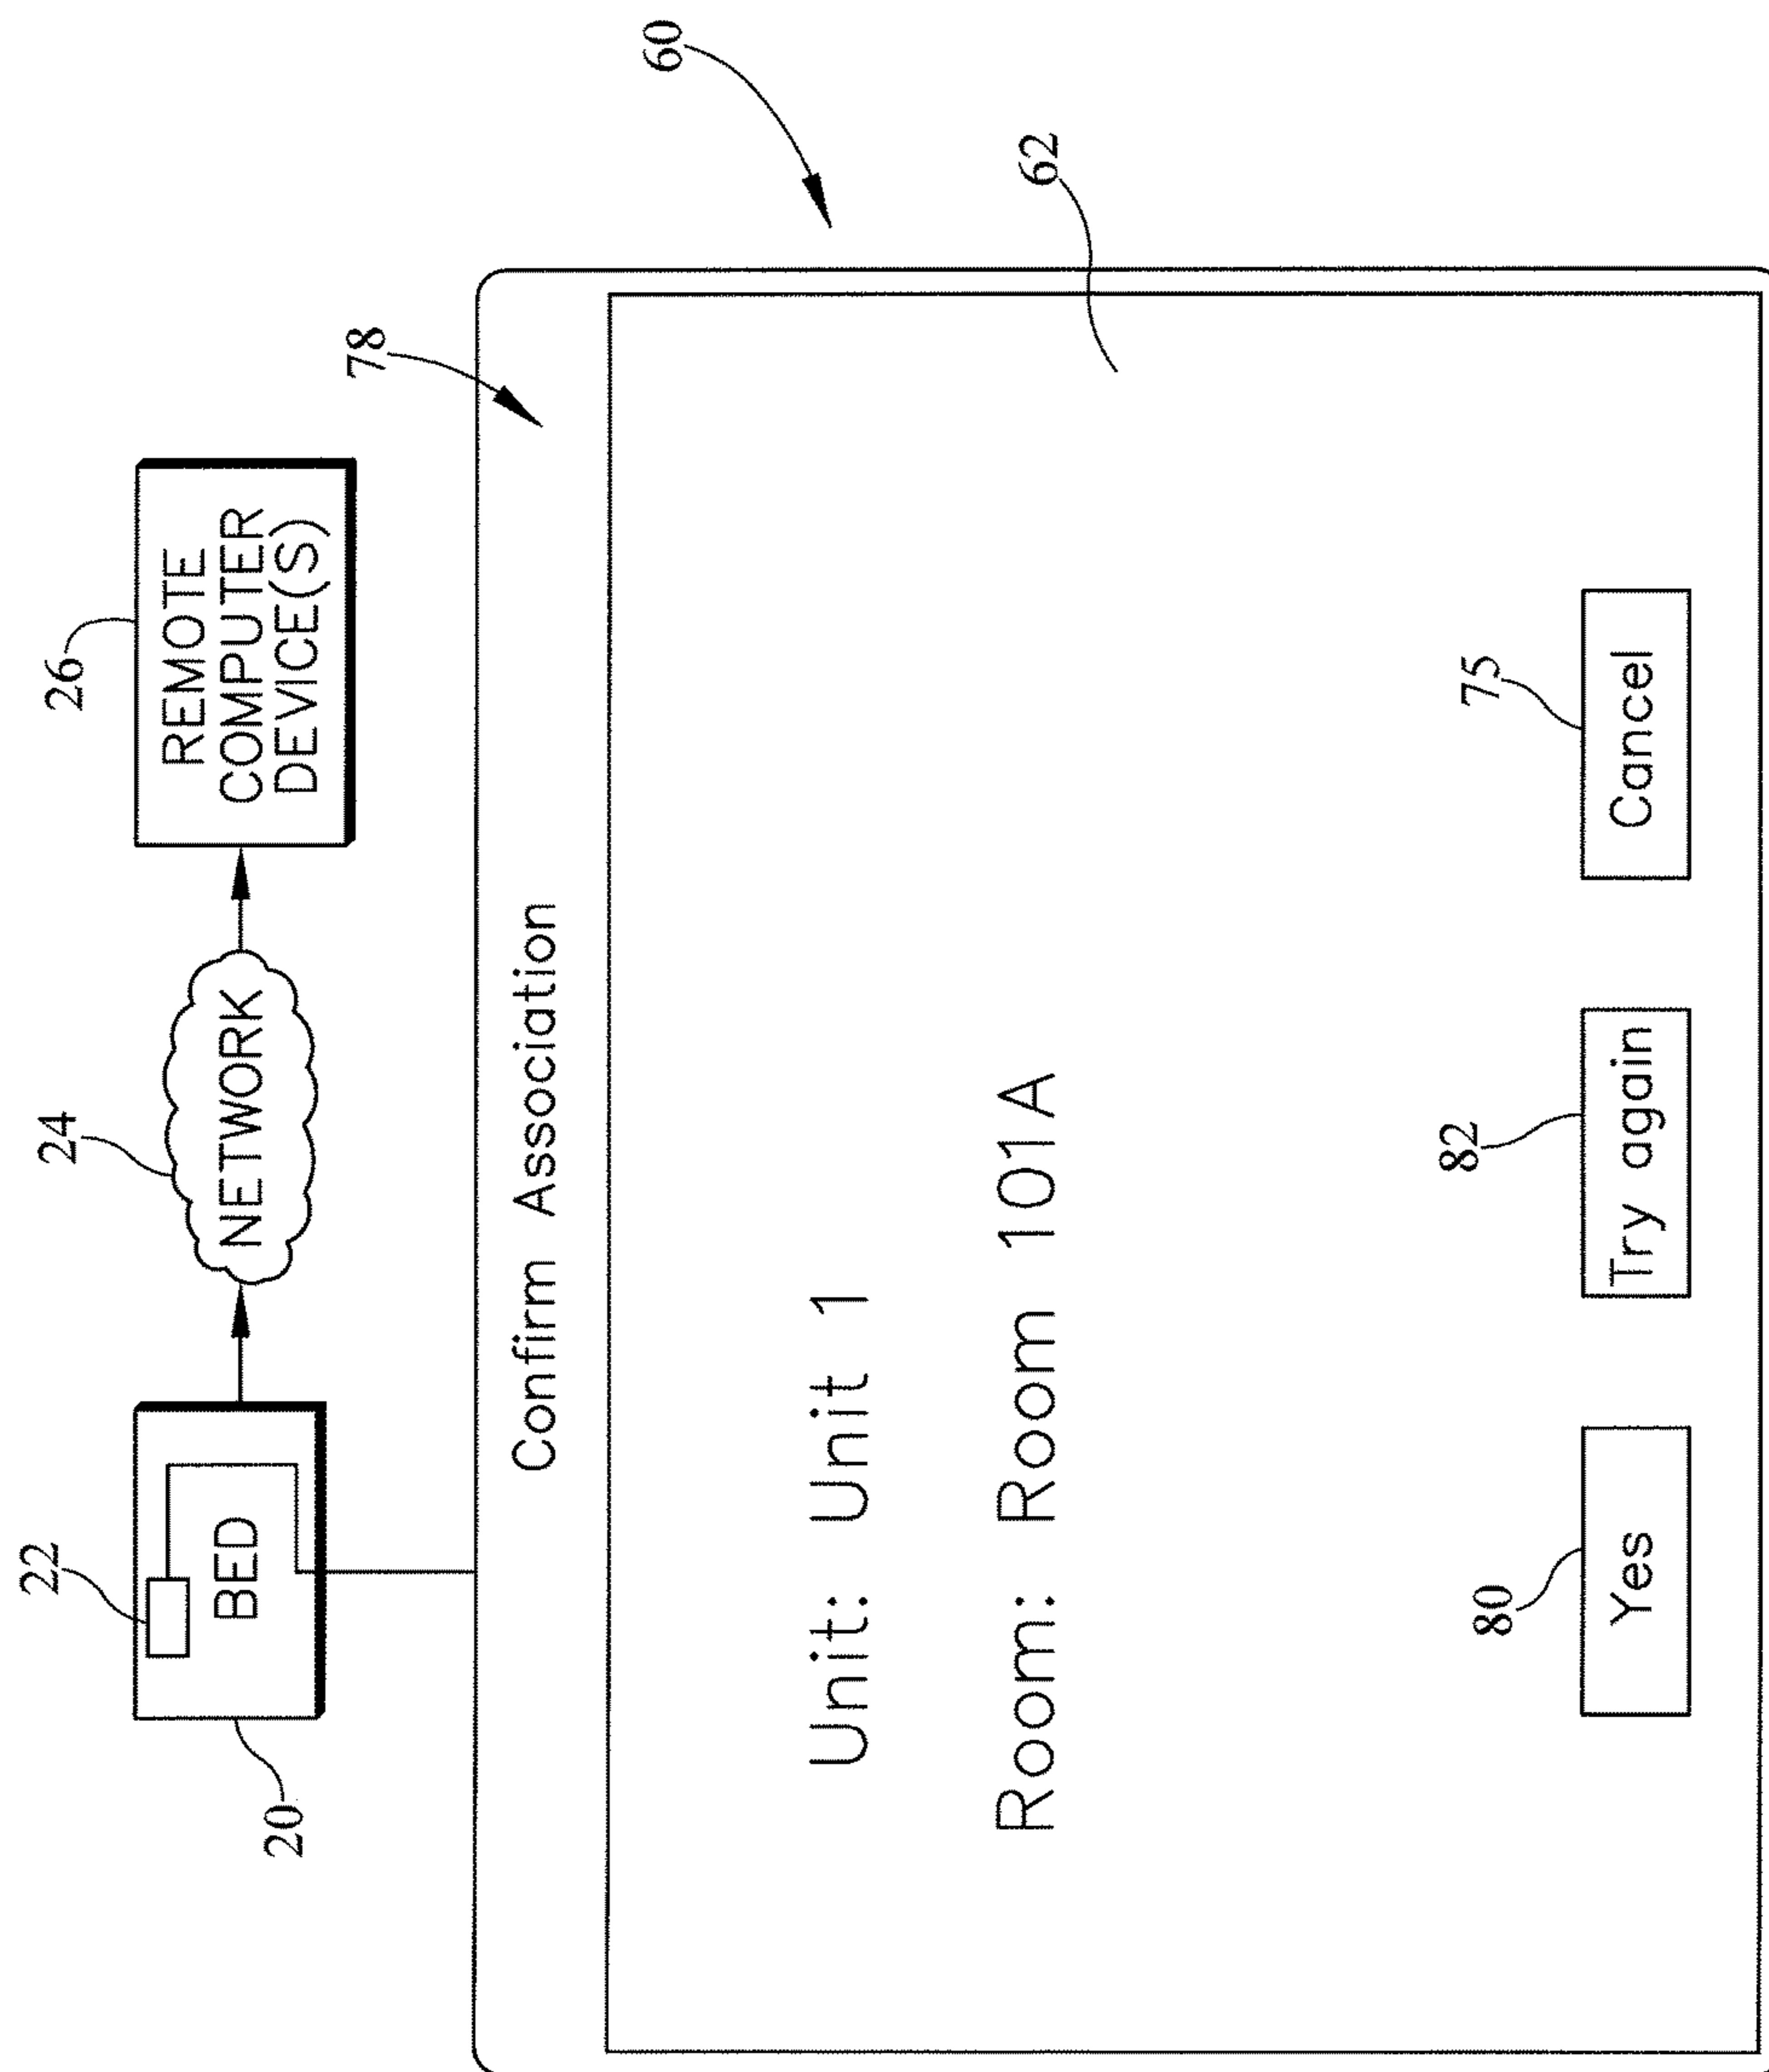


FIG. 10

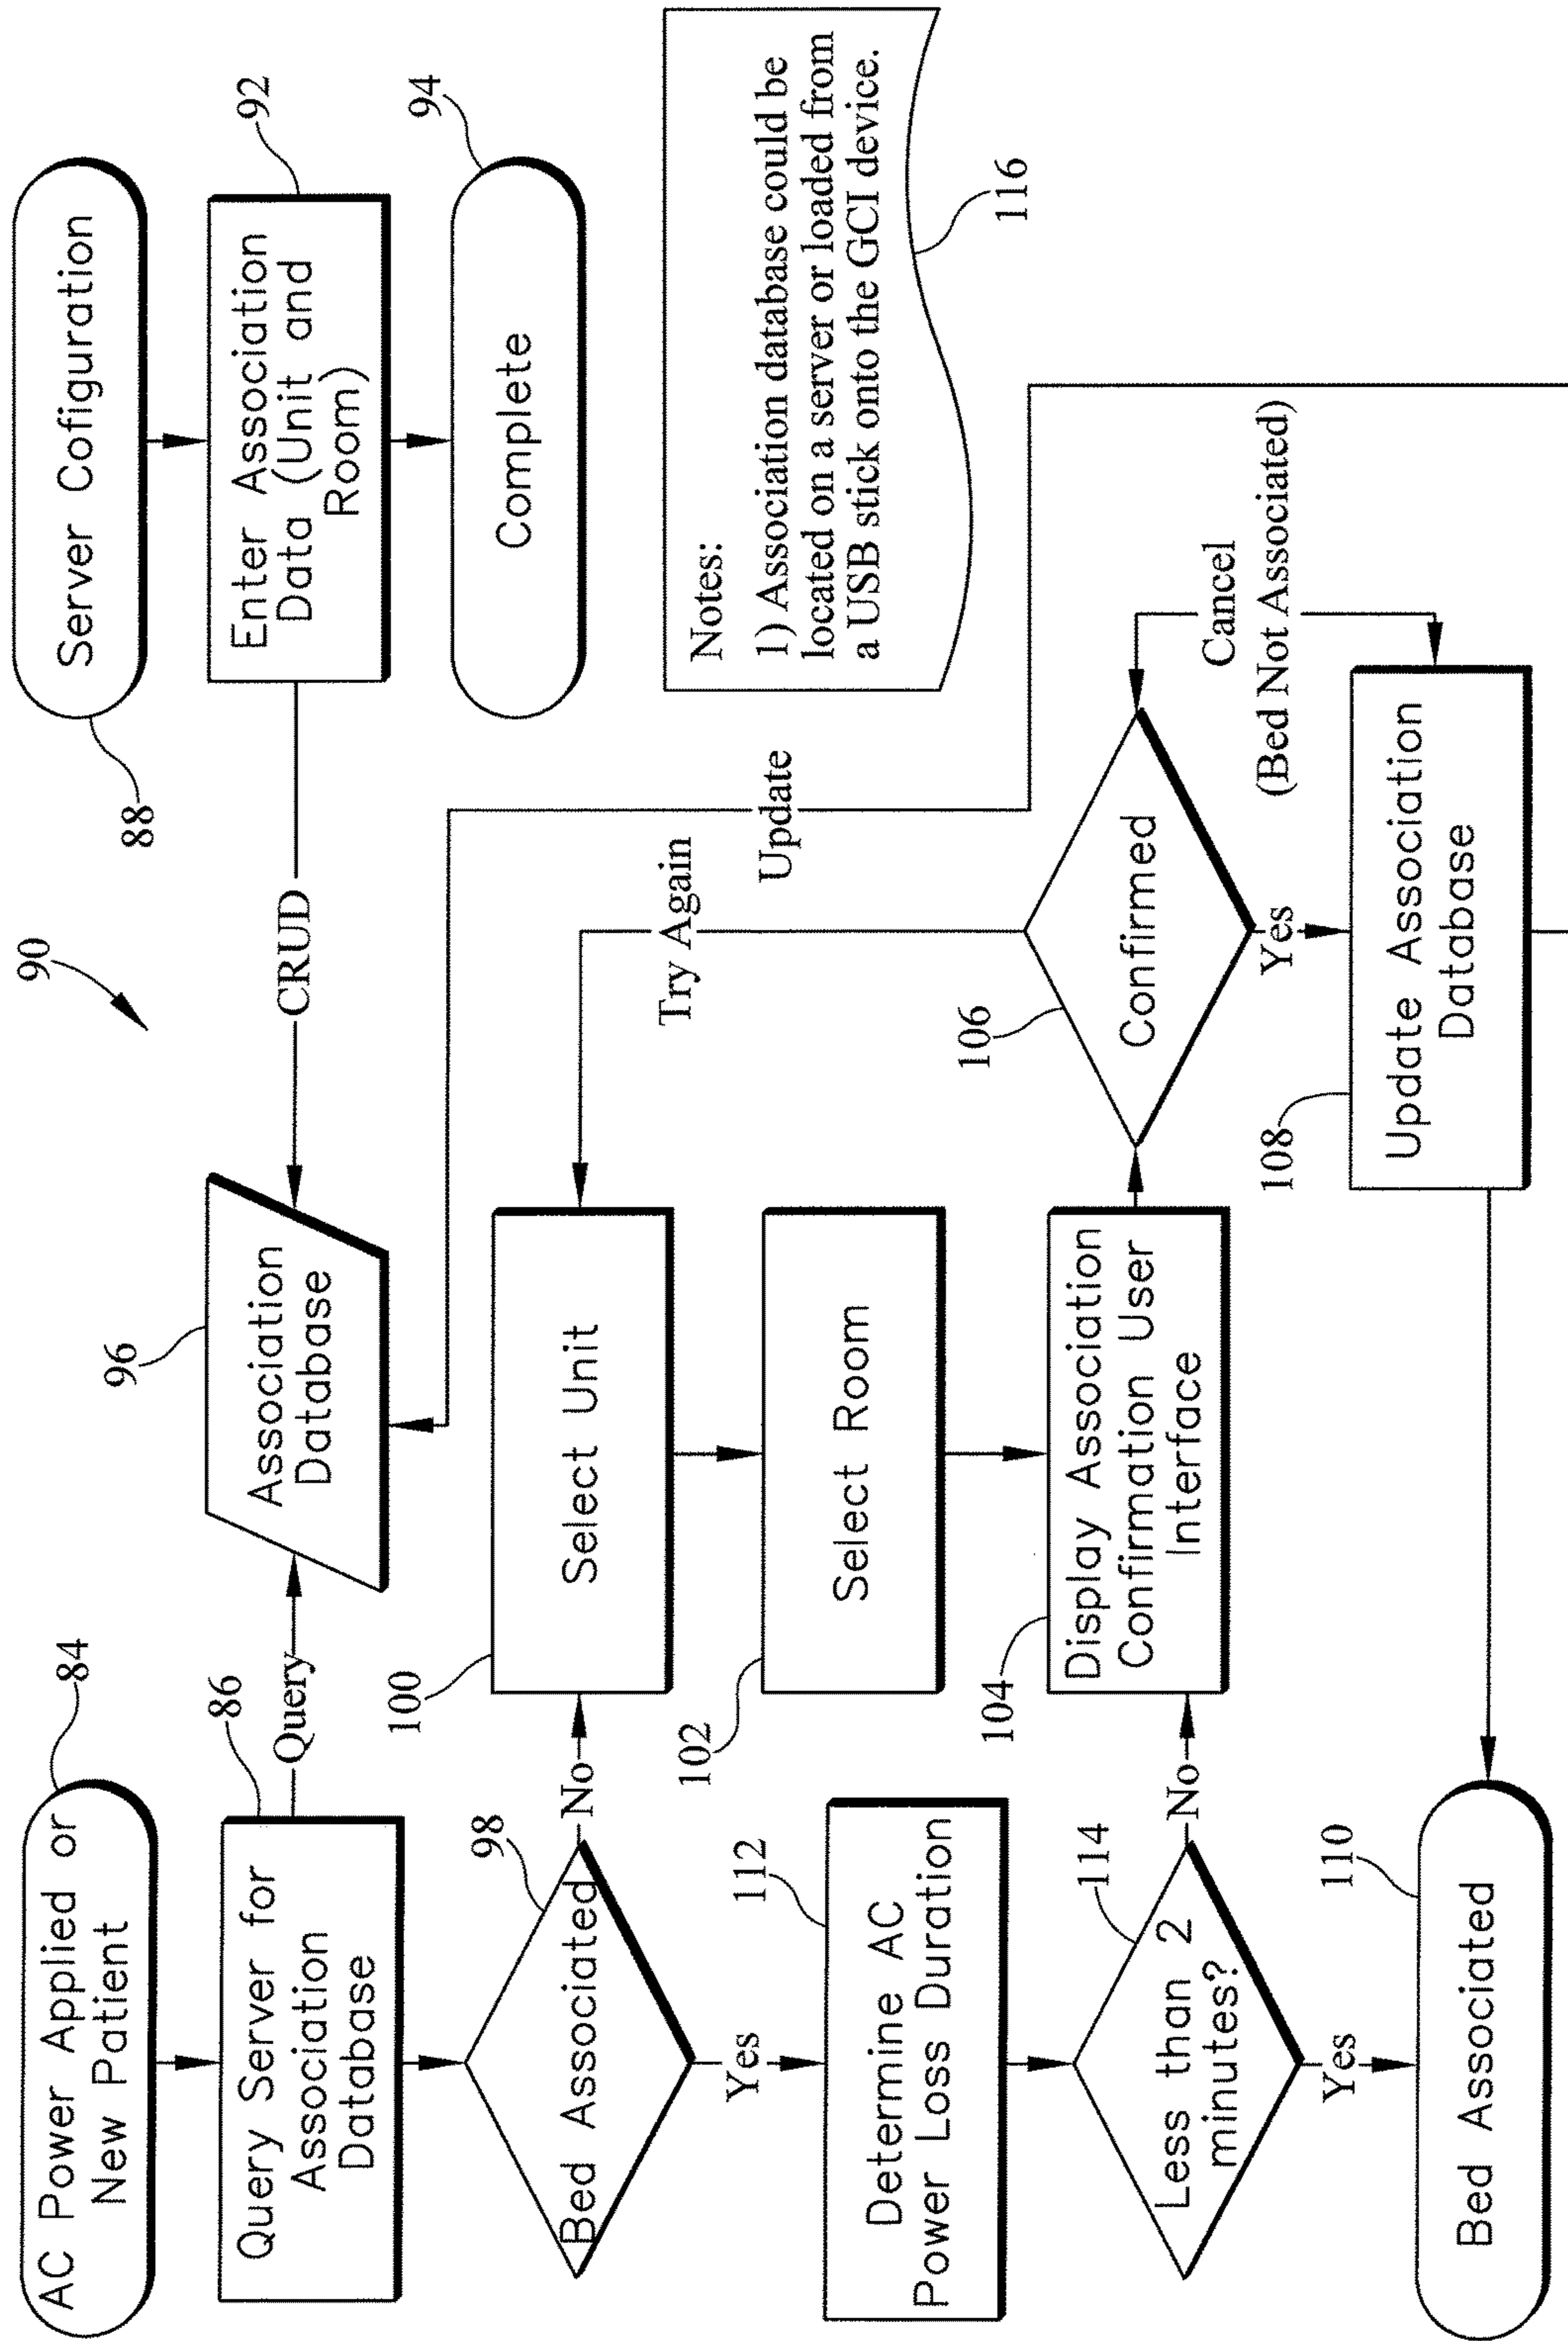


FIG. 11

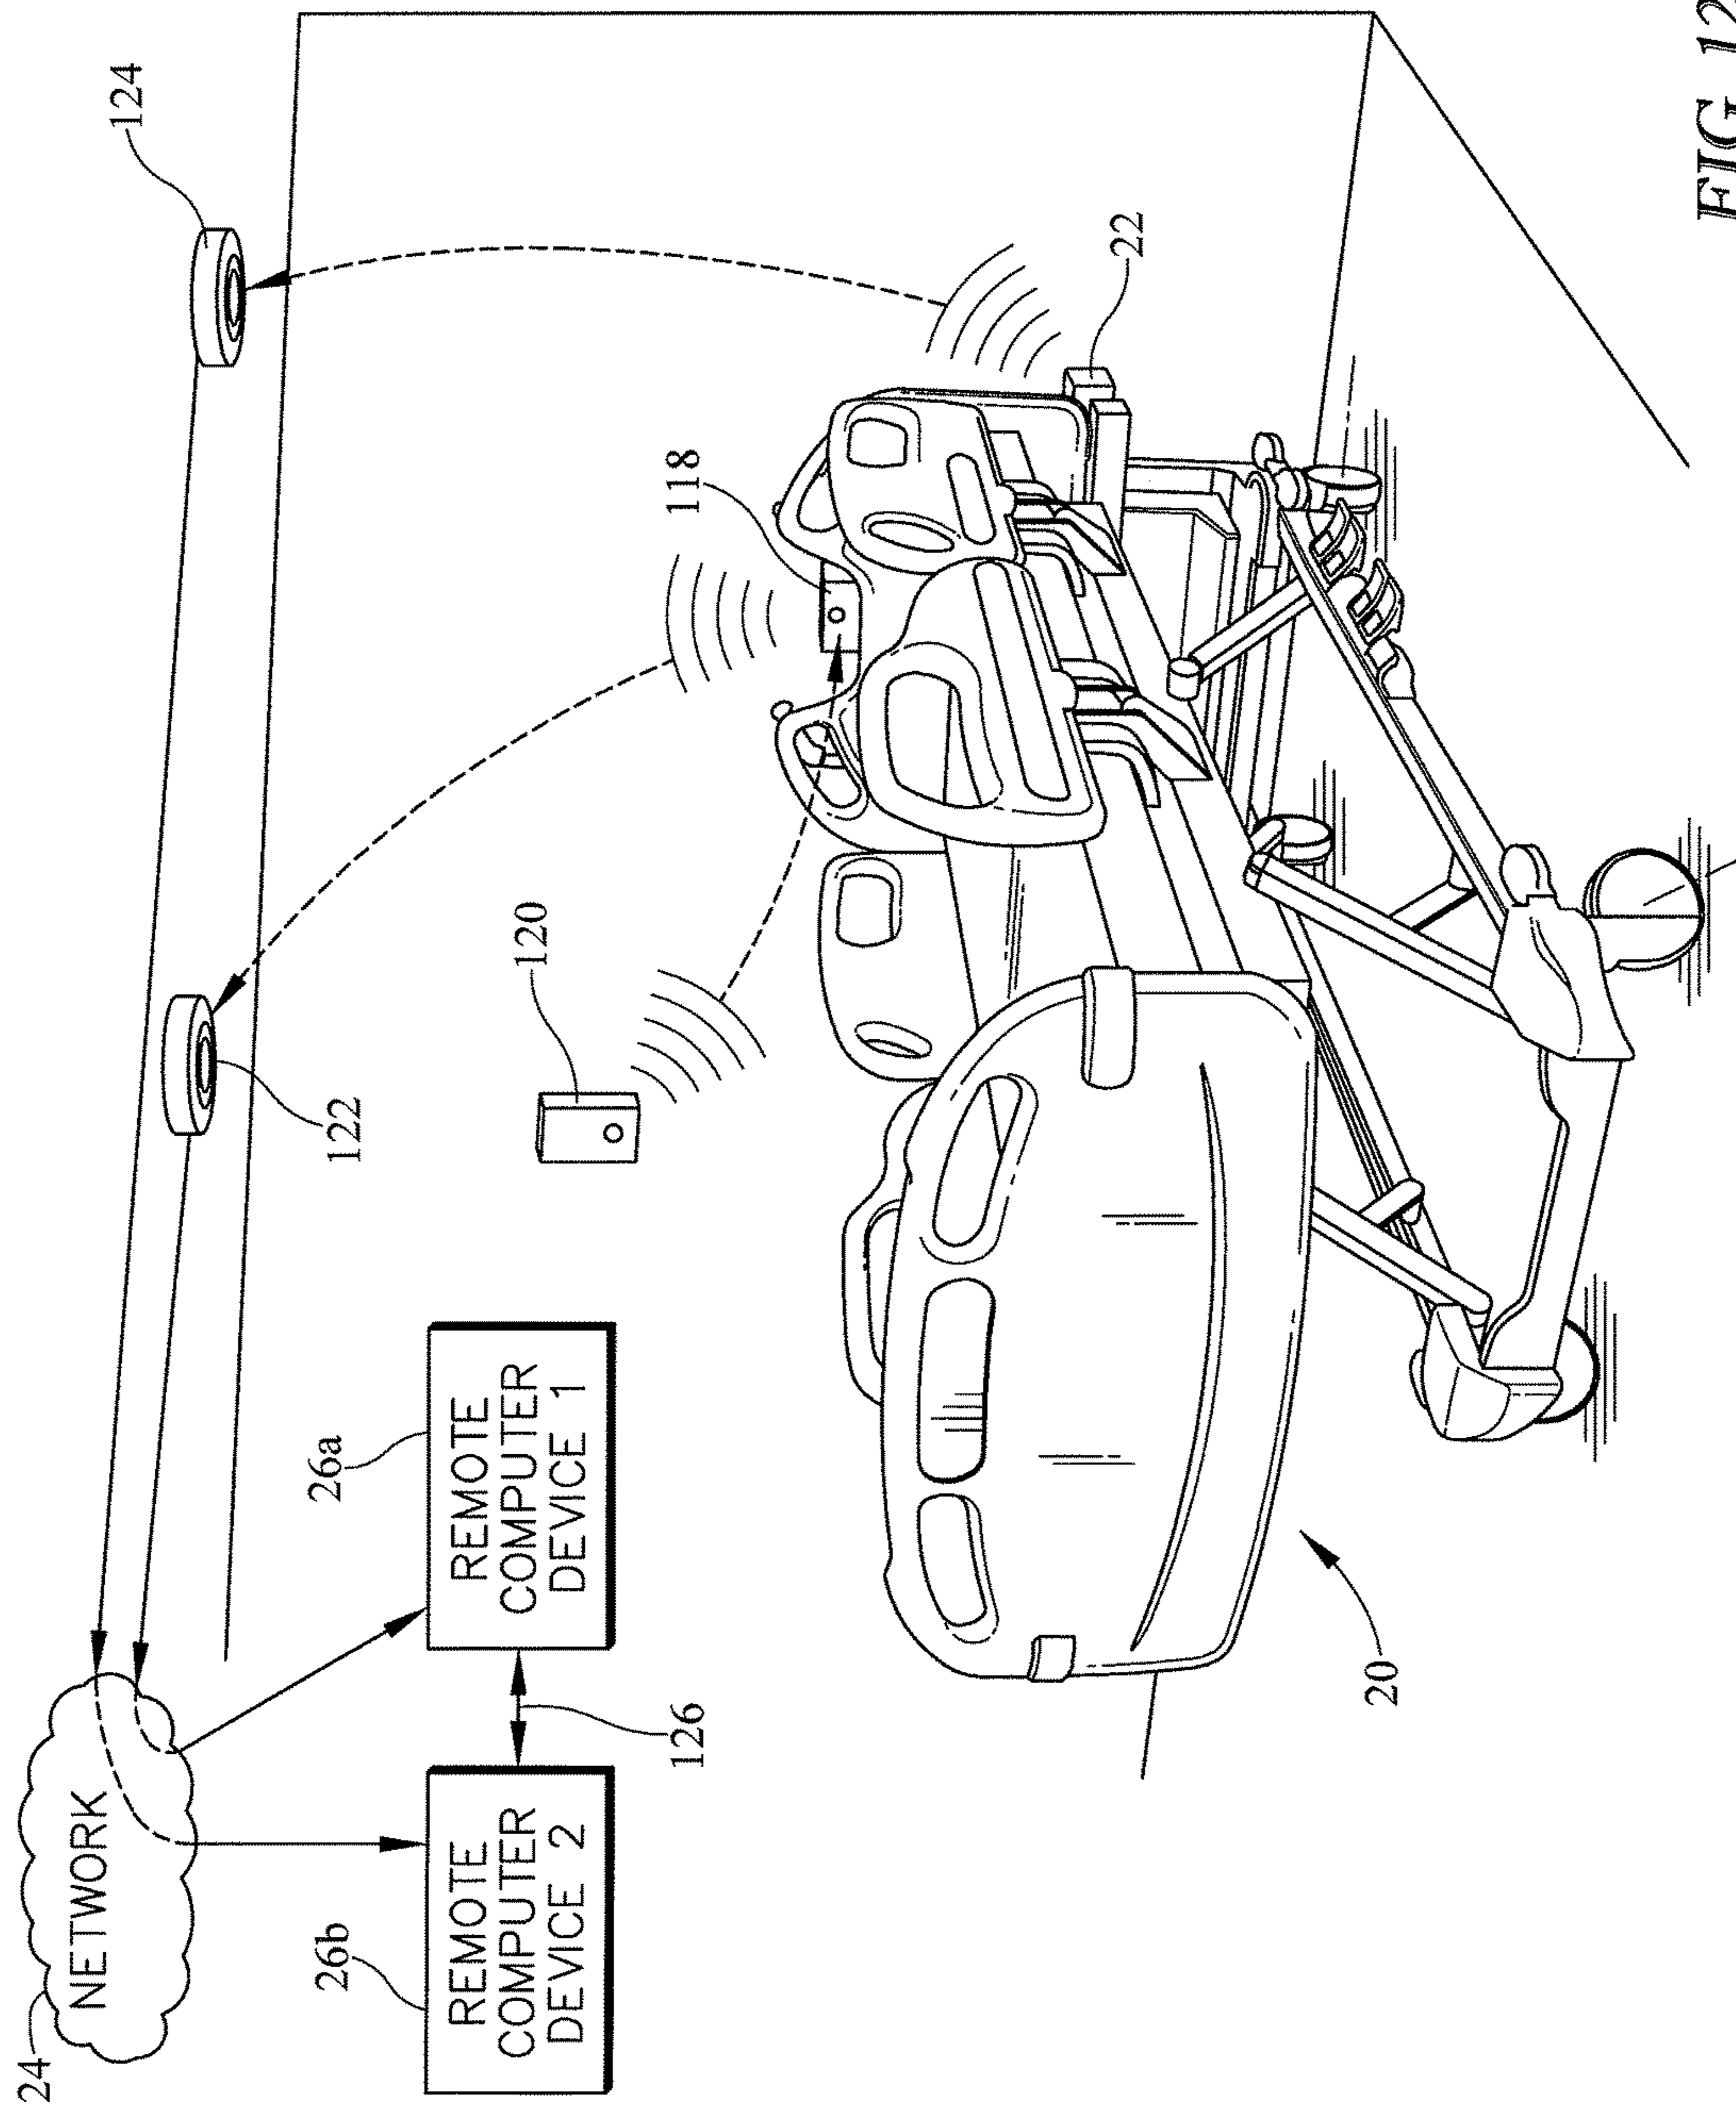


FIG. 12

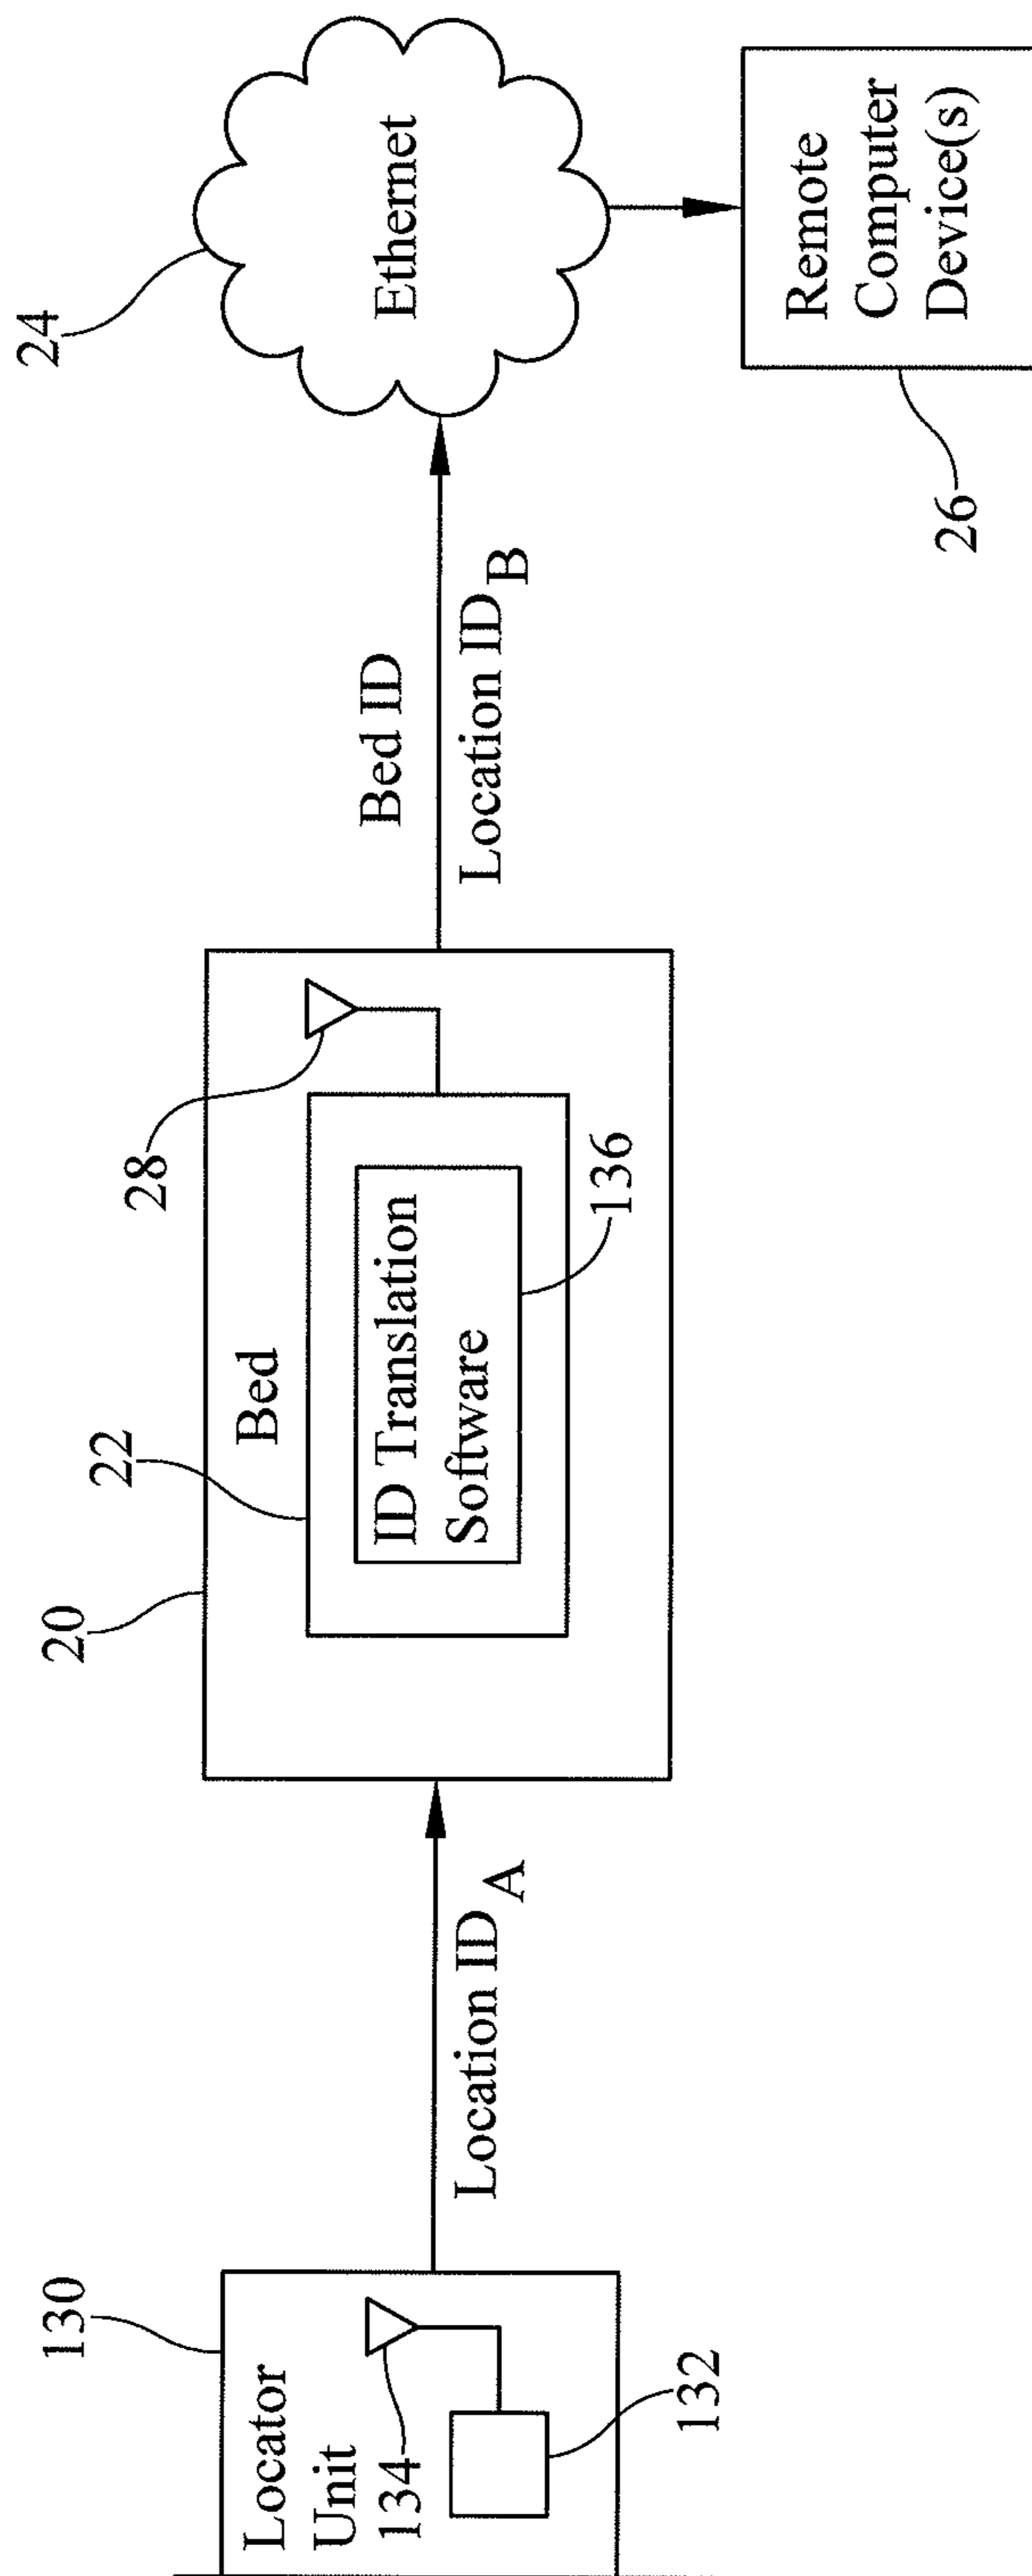


FIG. 13

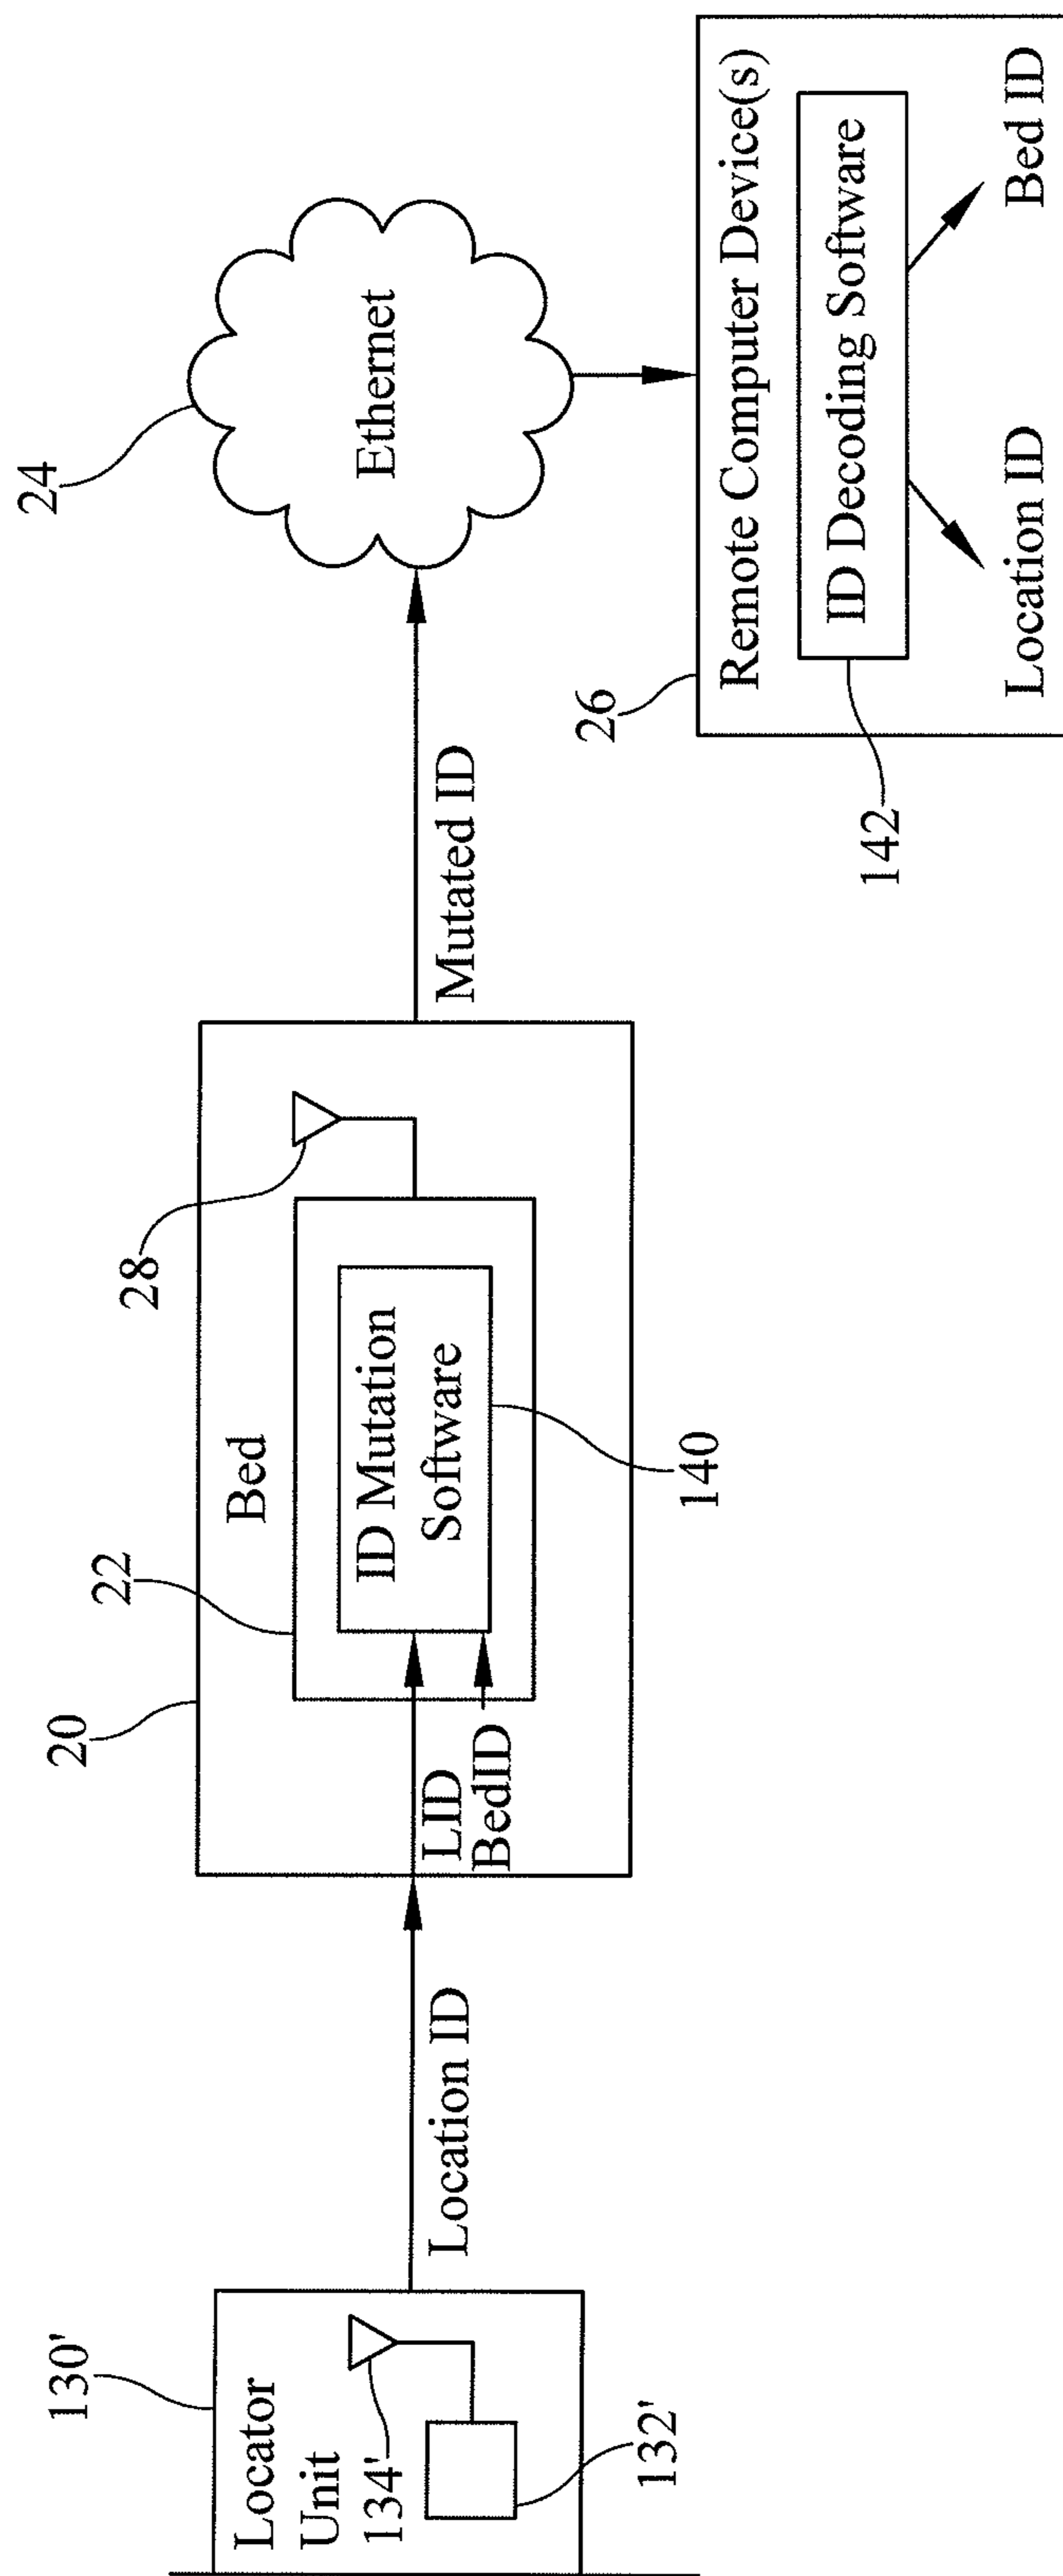
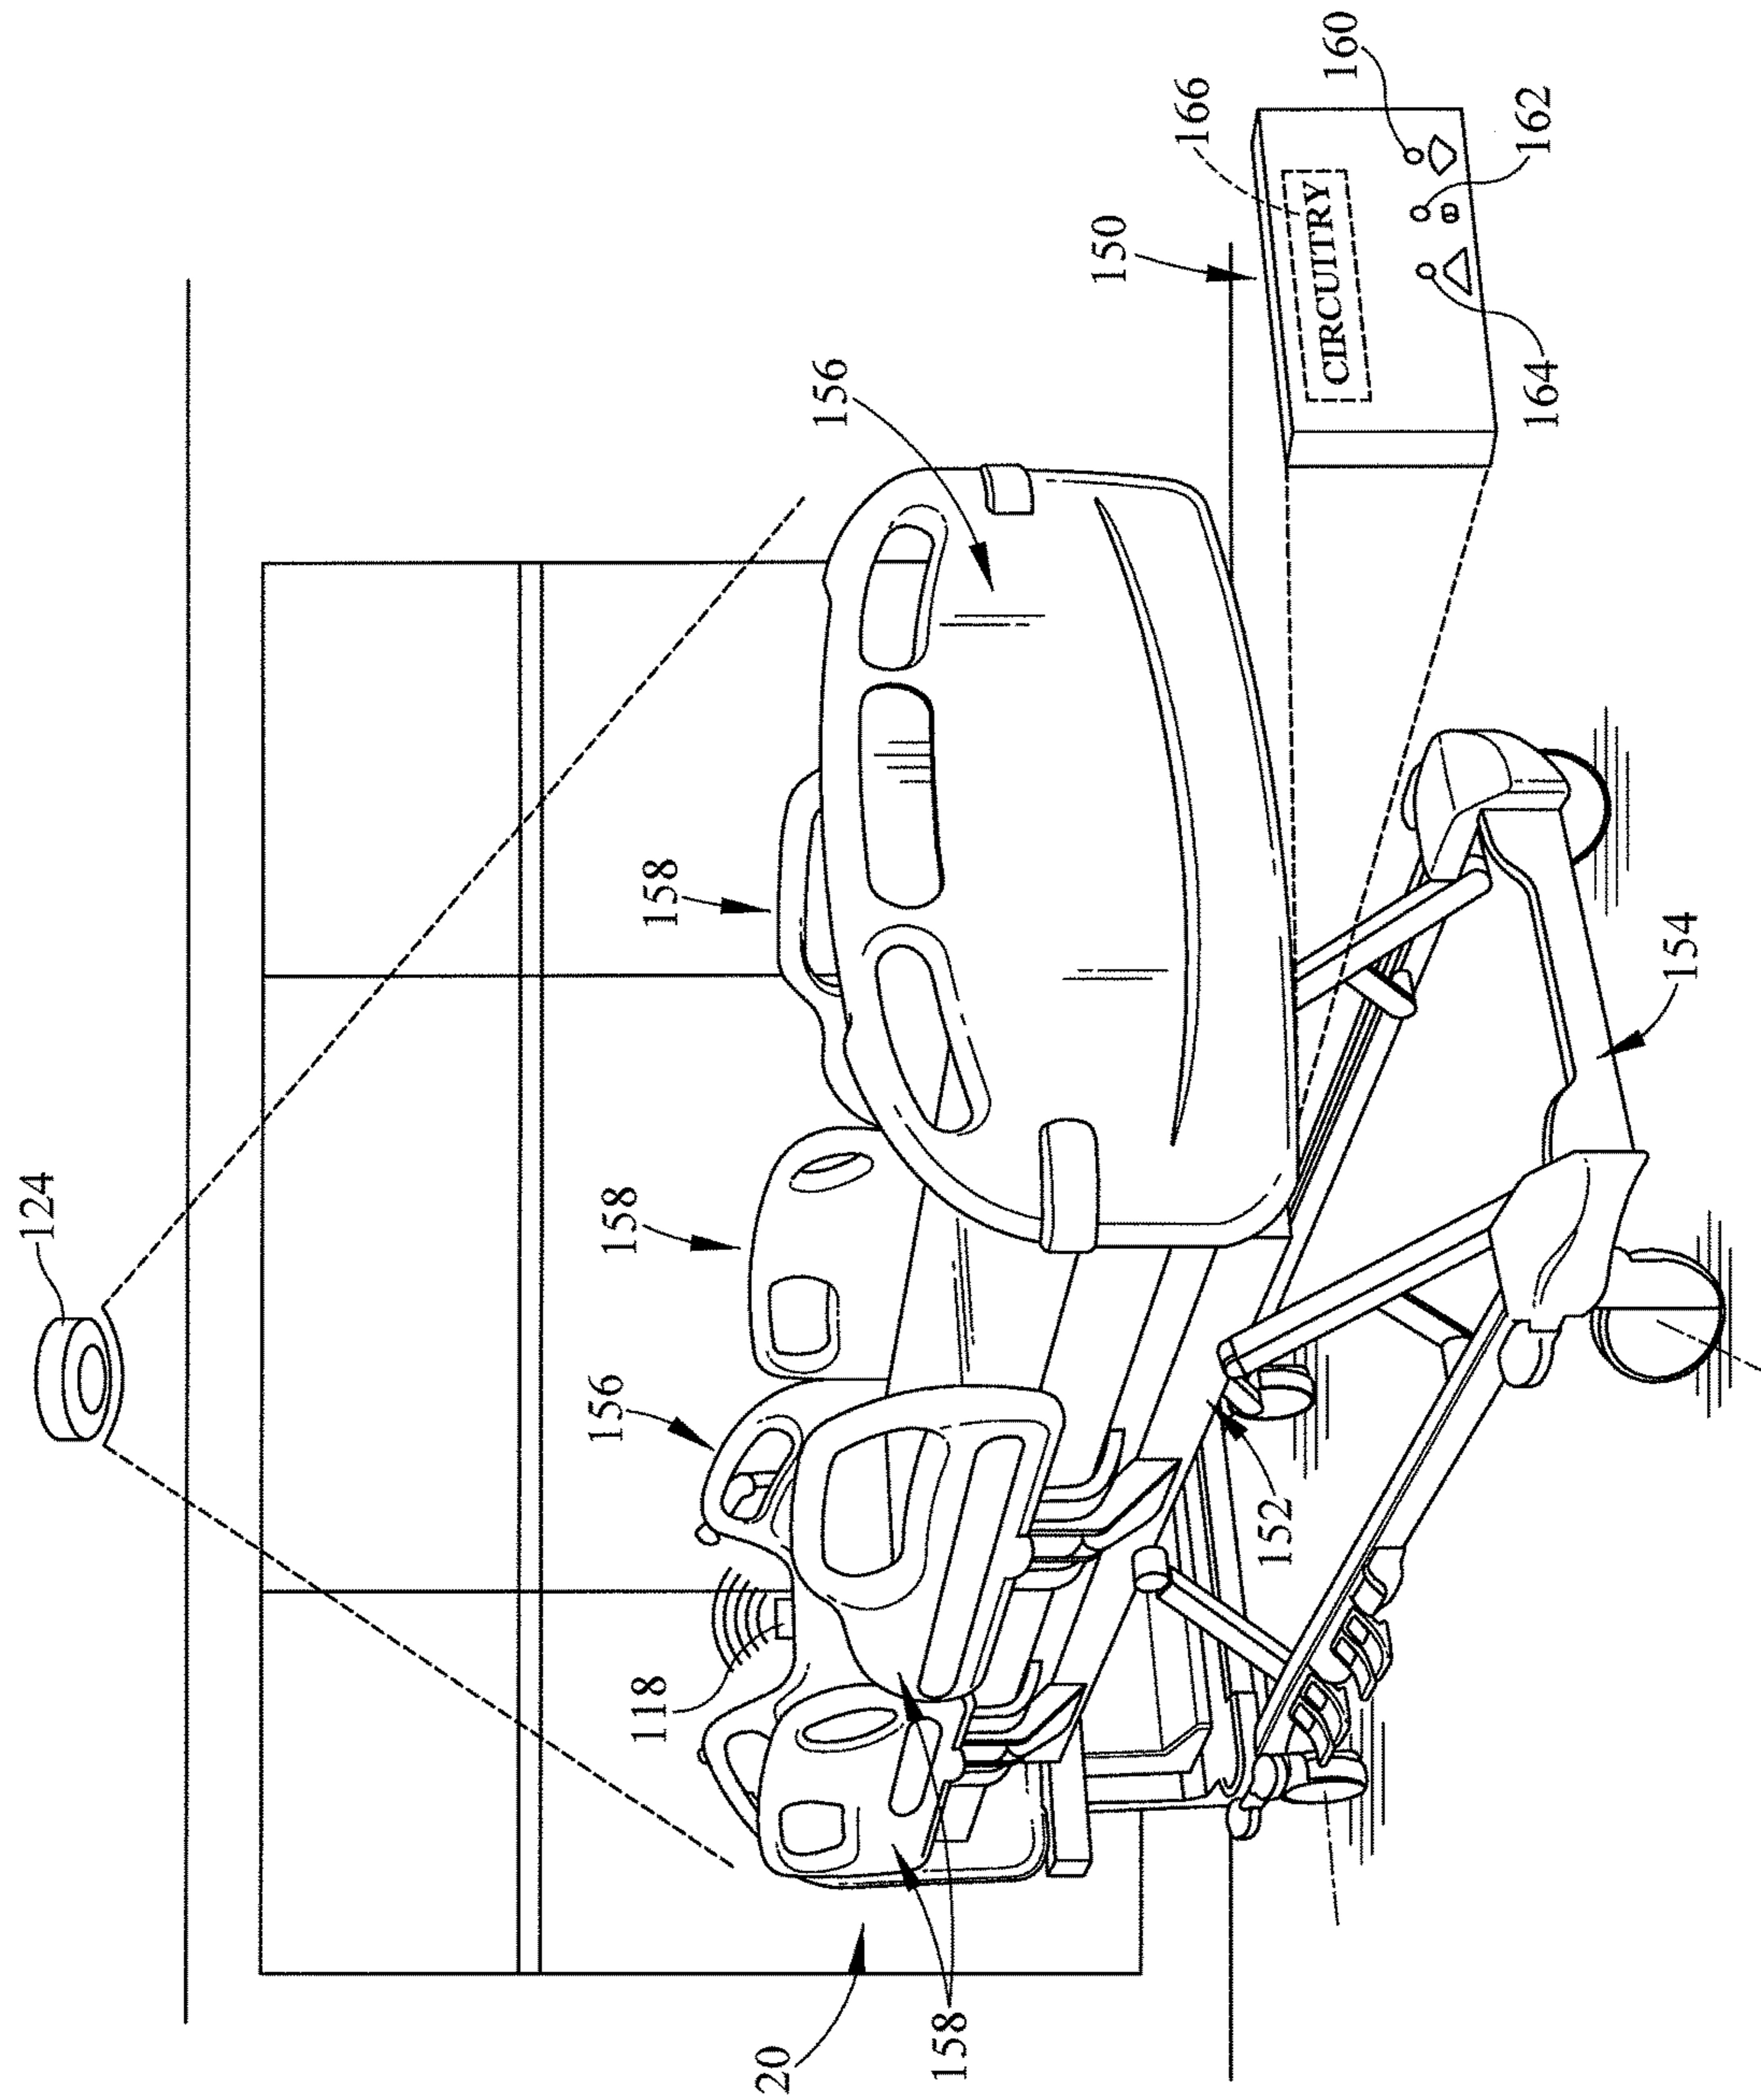


FIG. 14



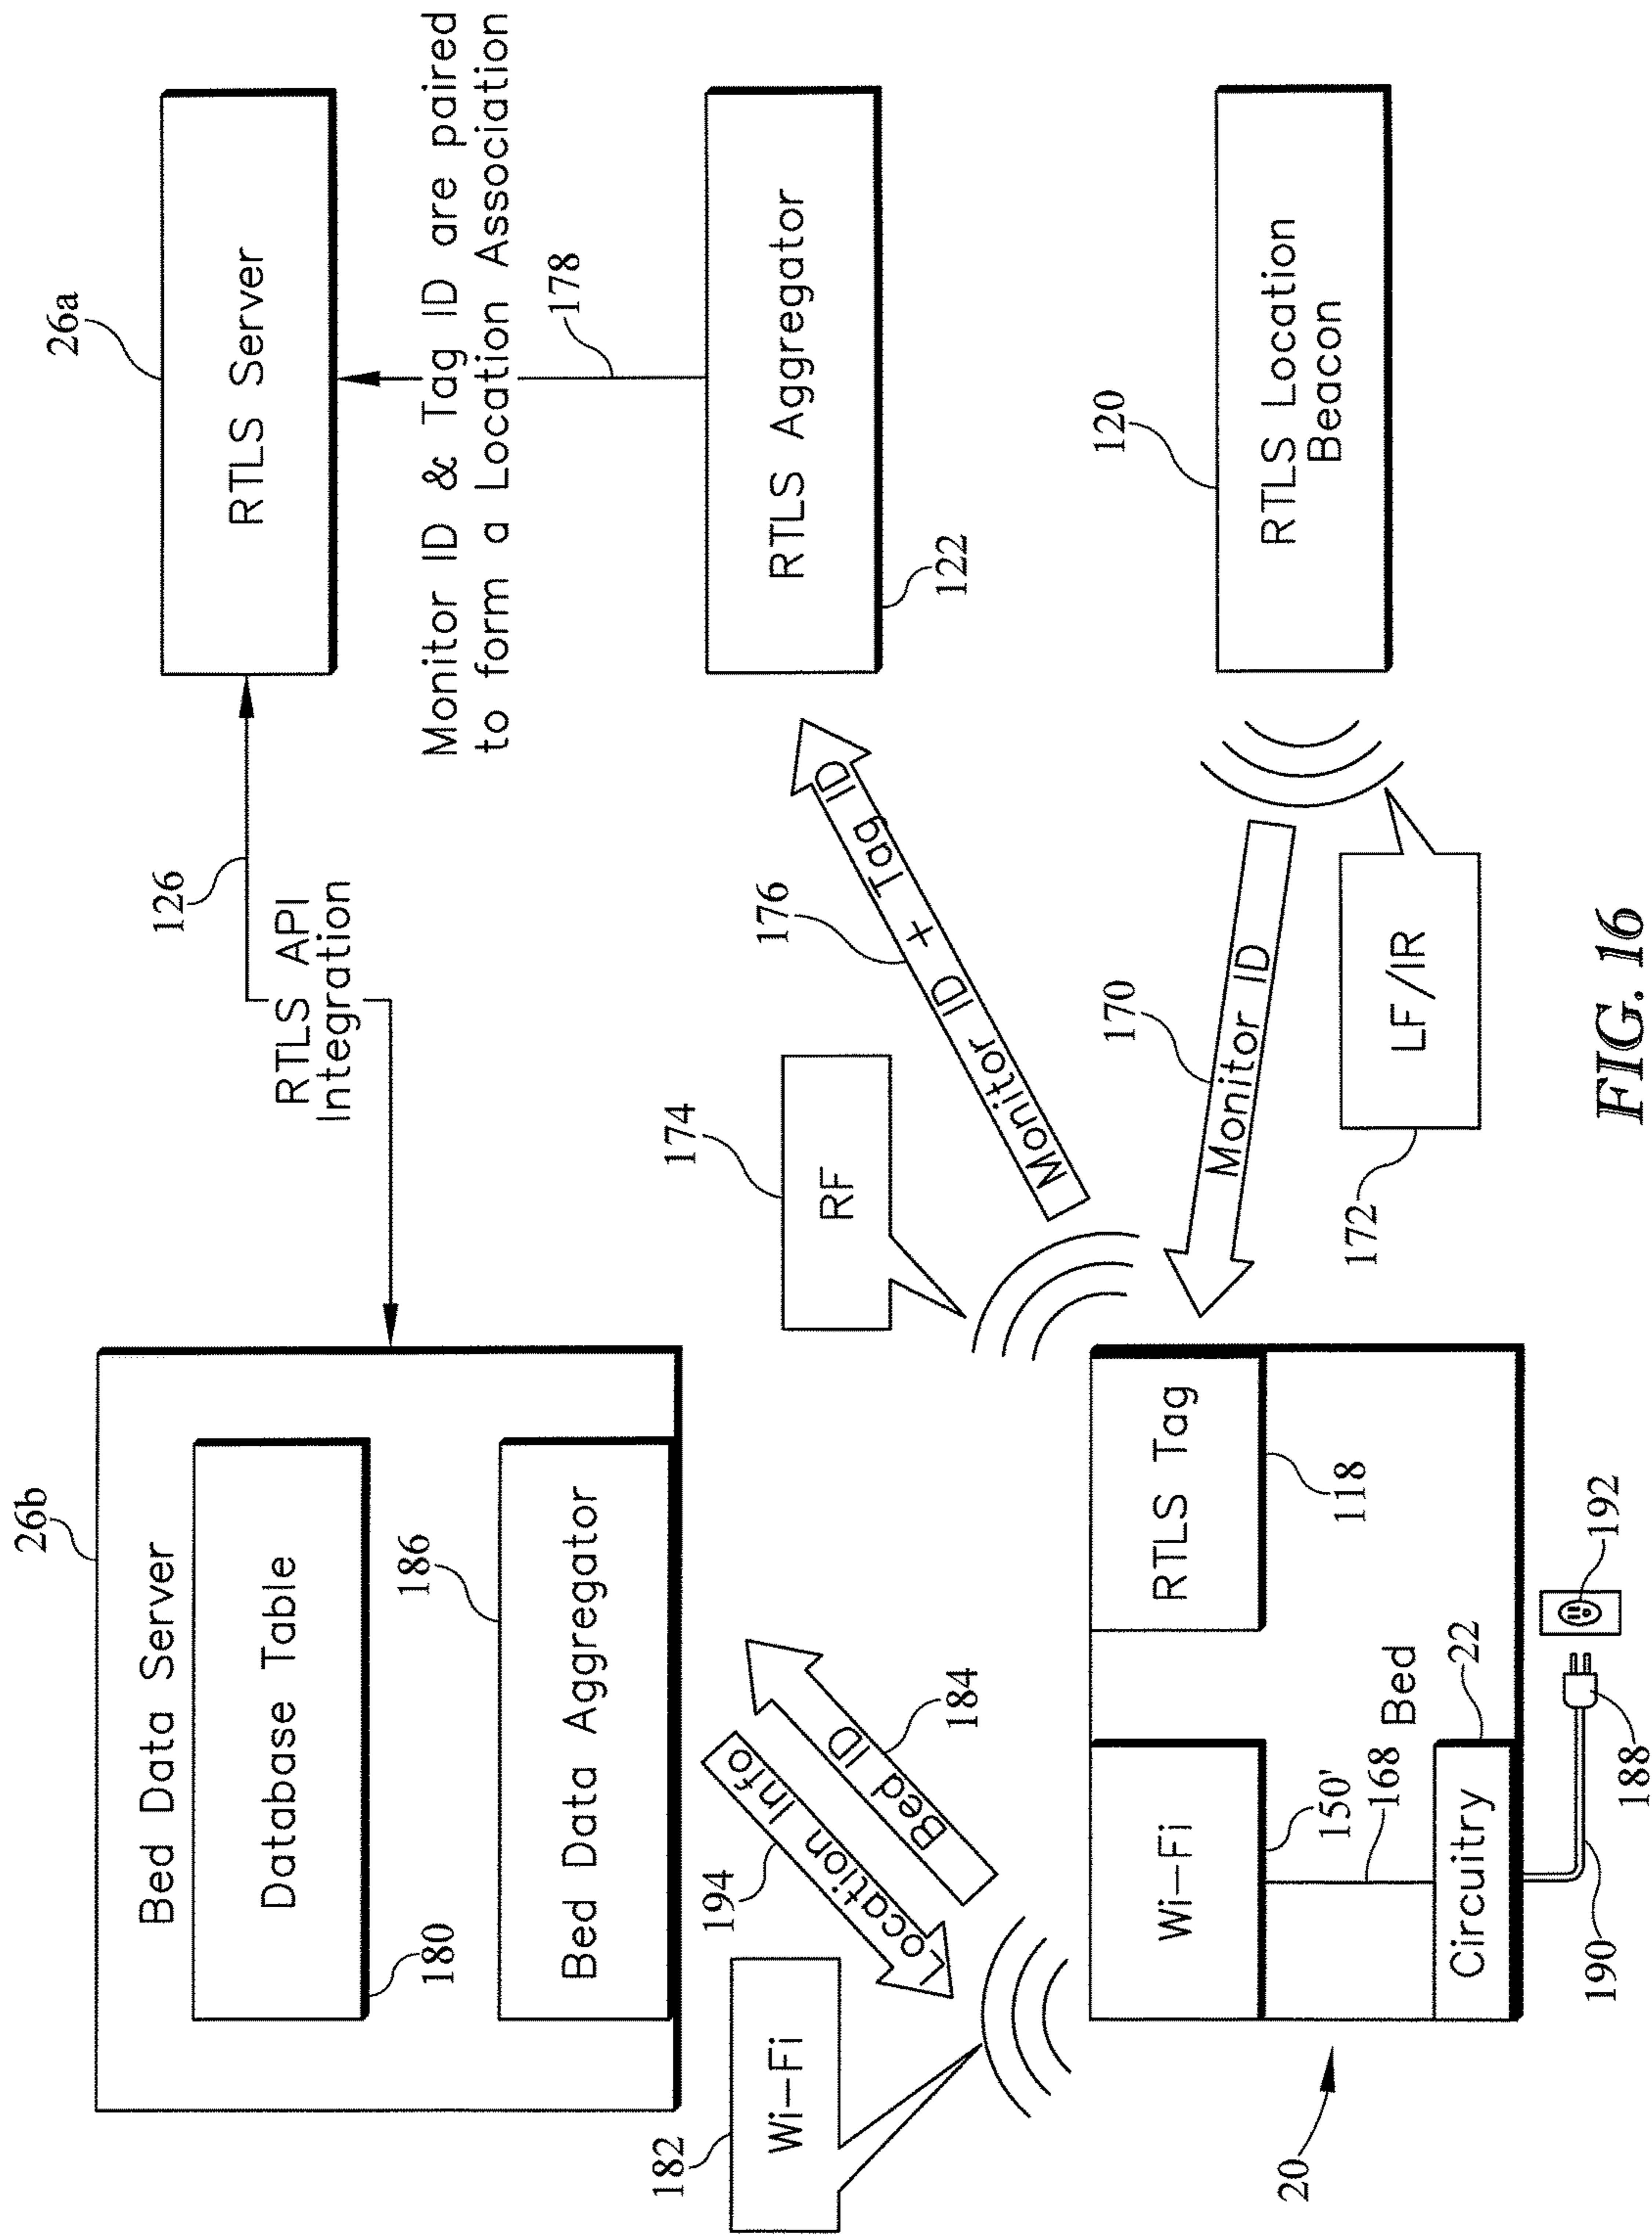


FIG. 16

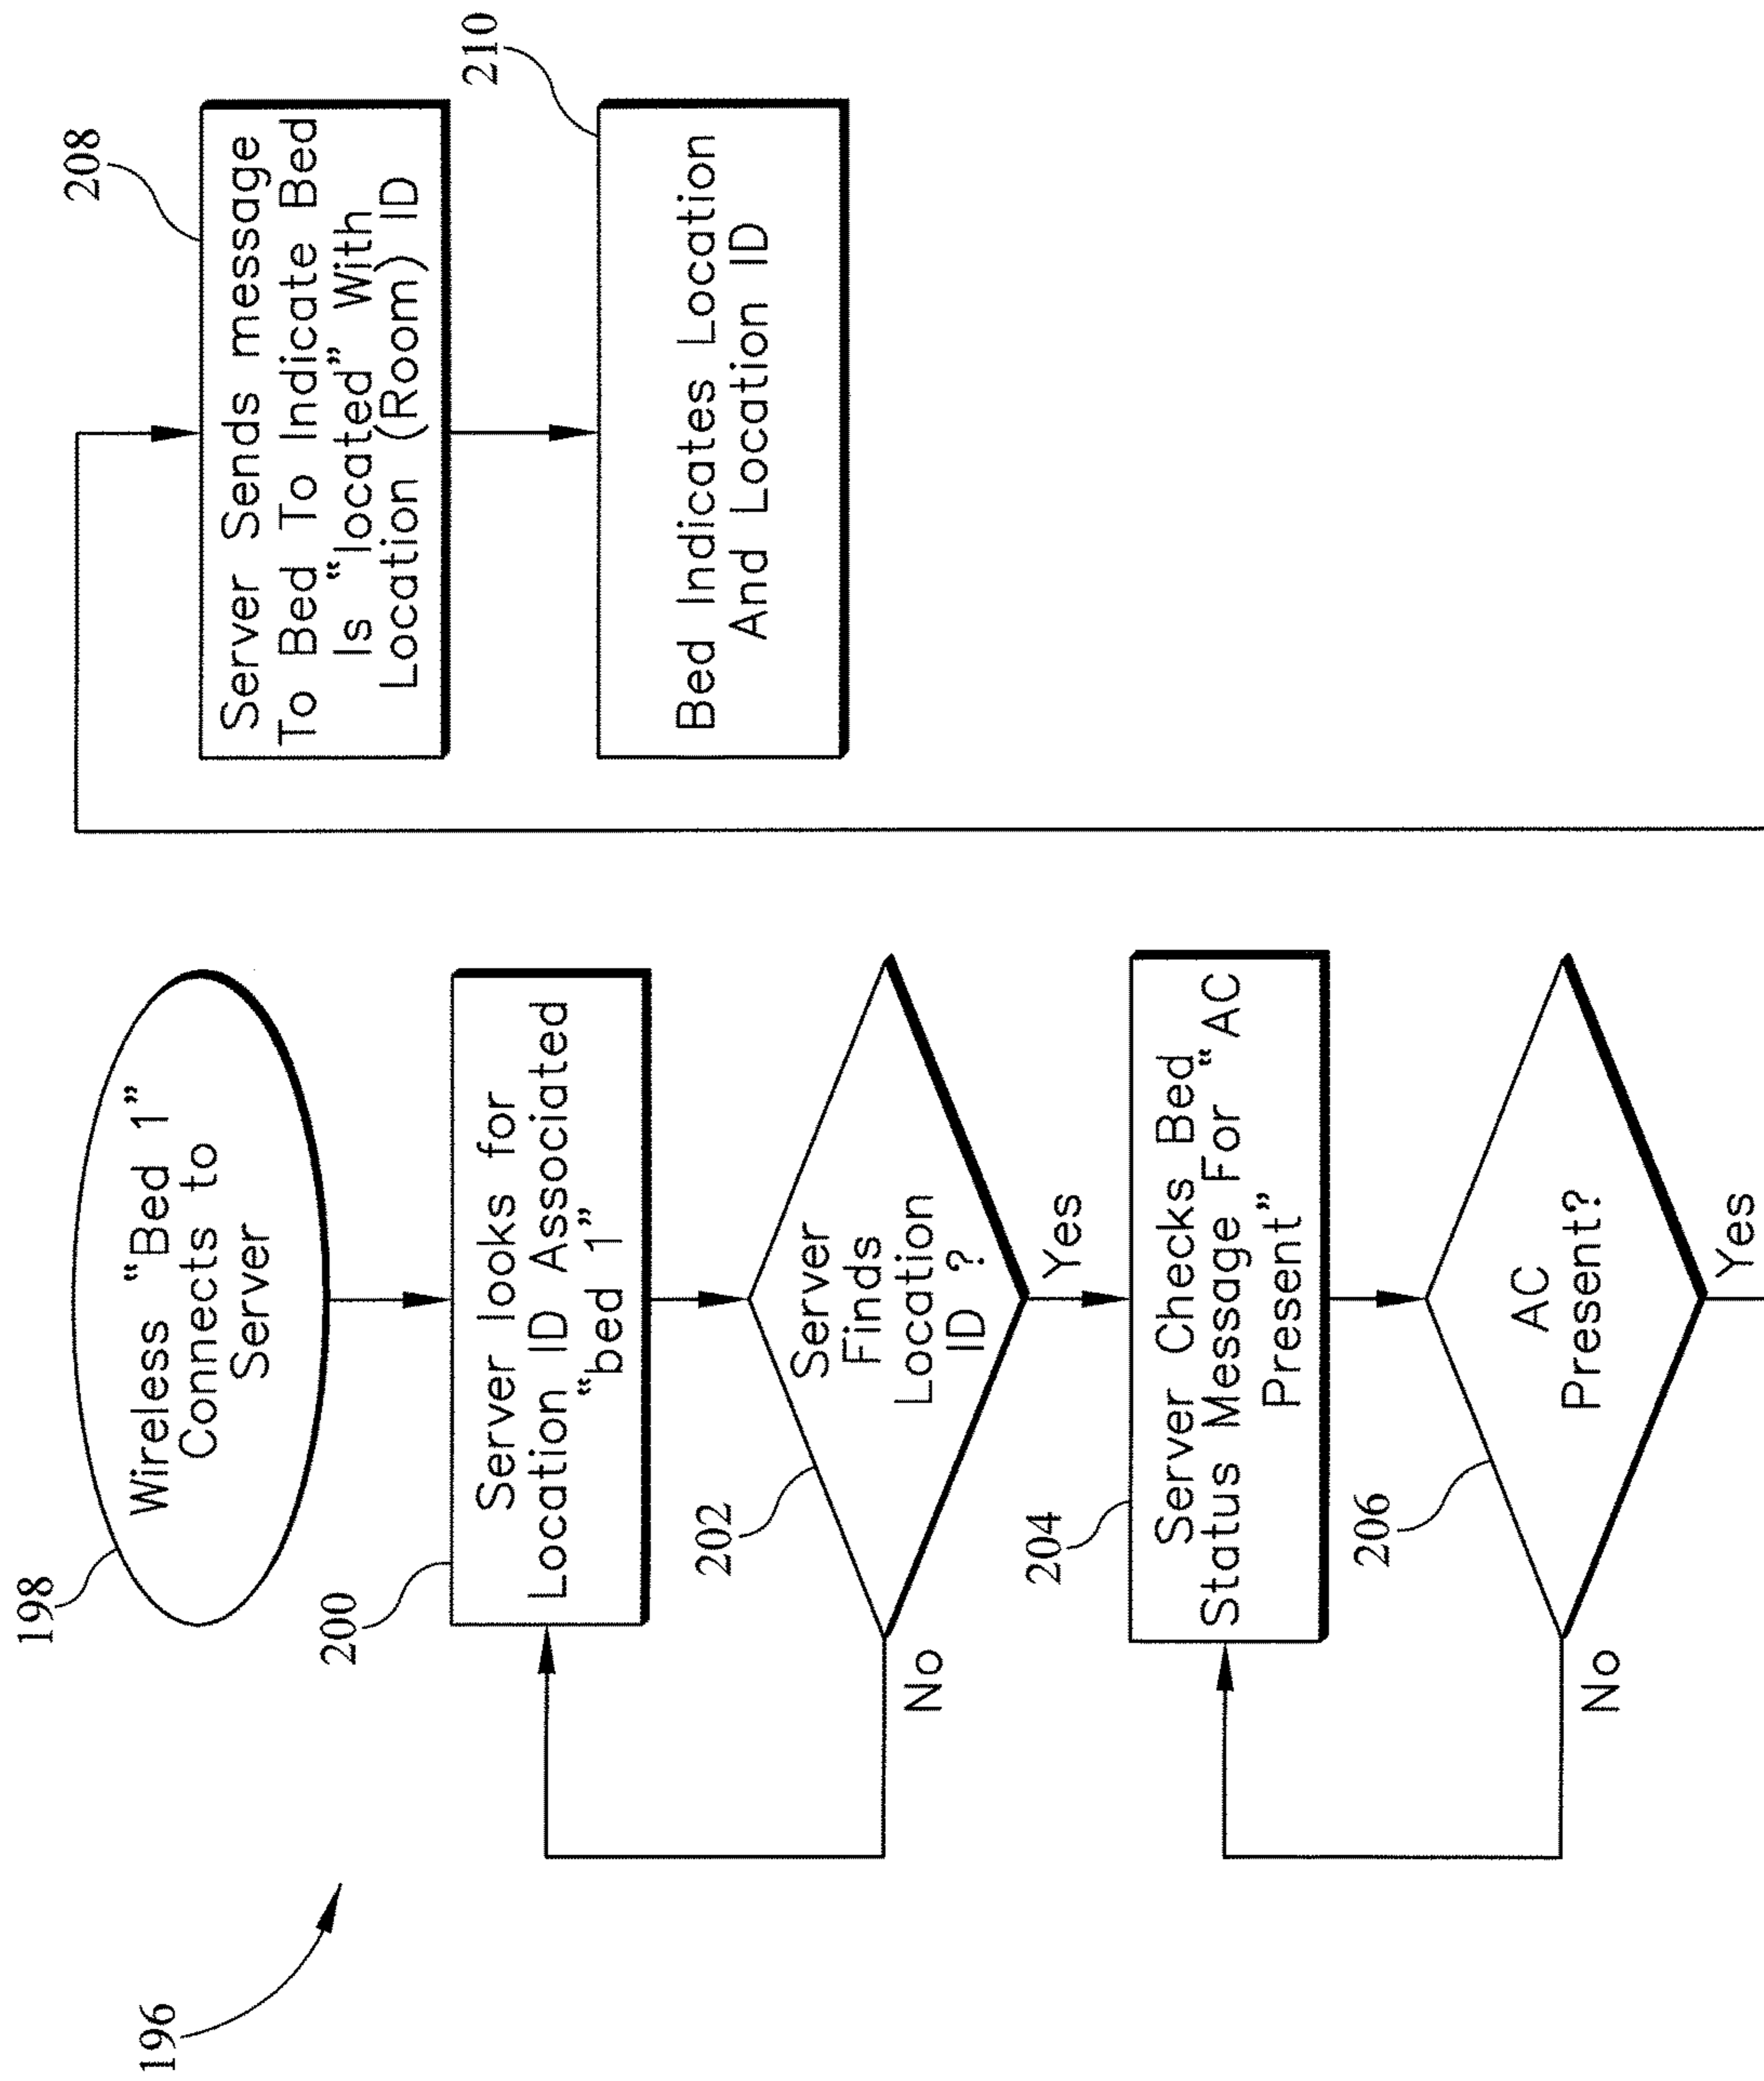


FIG. 17

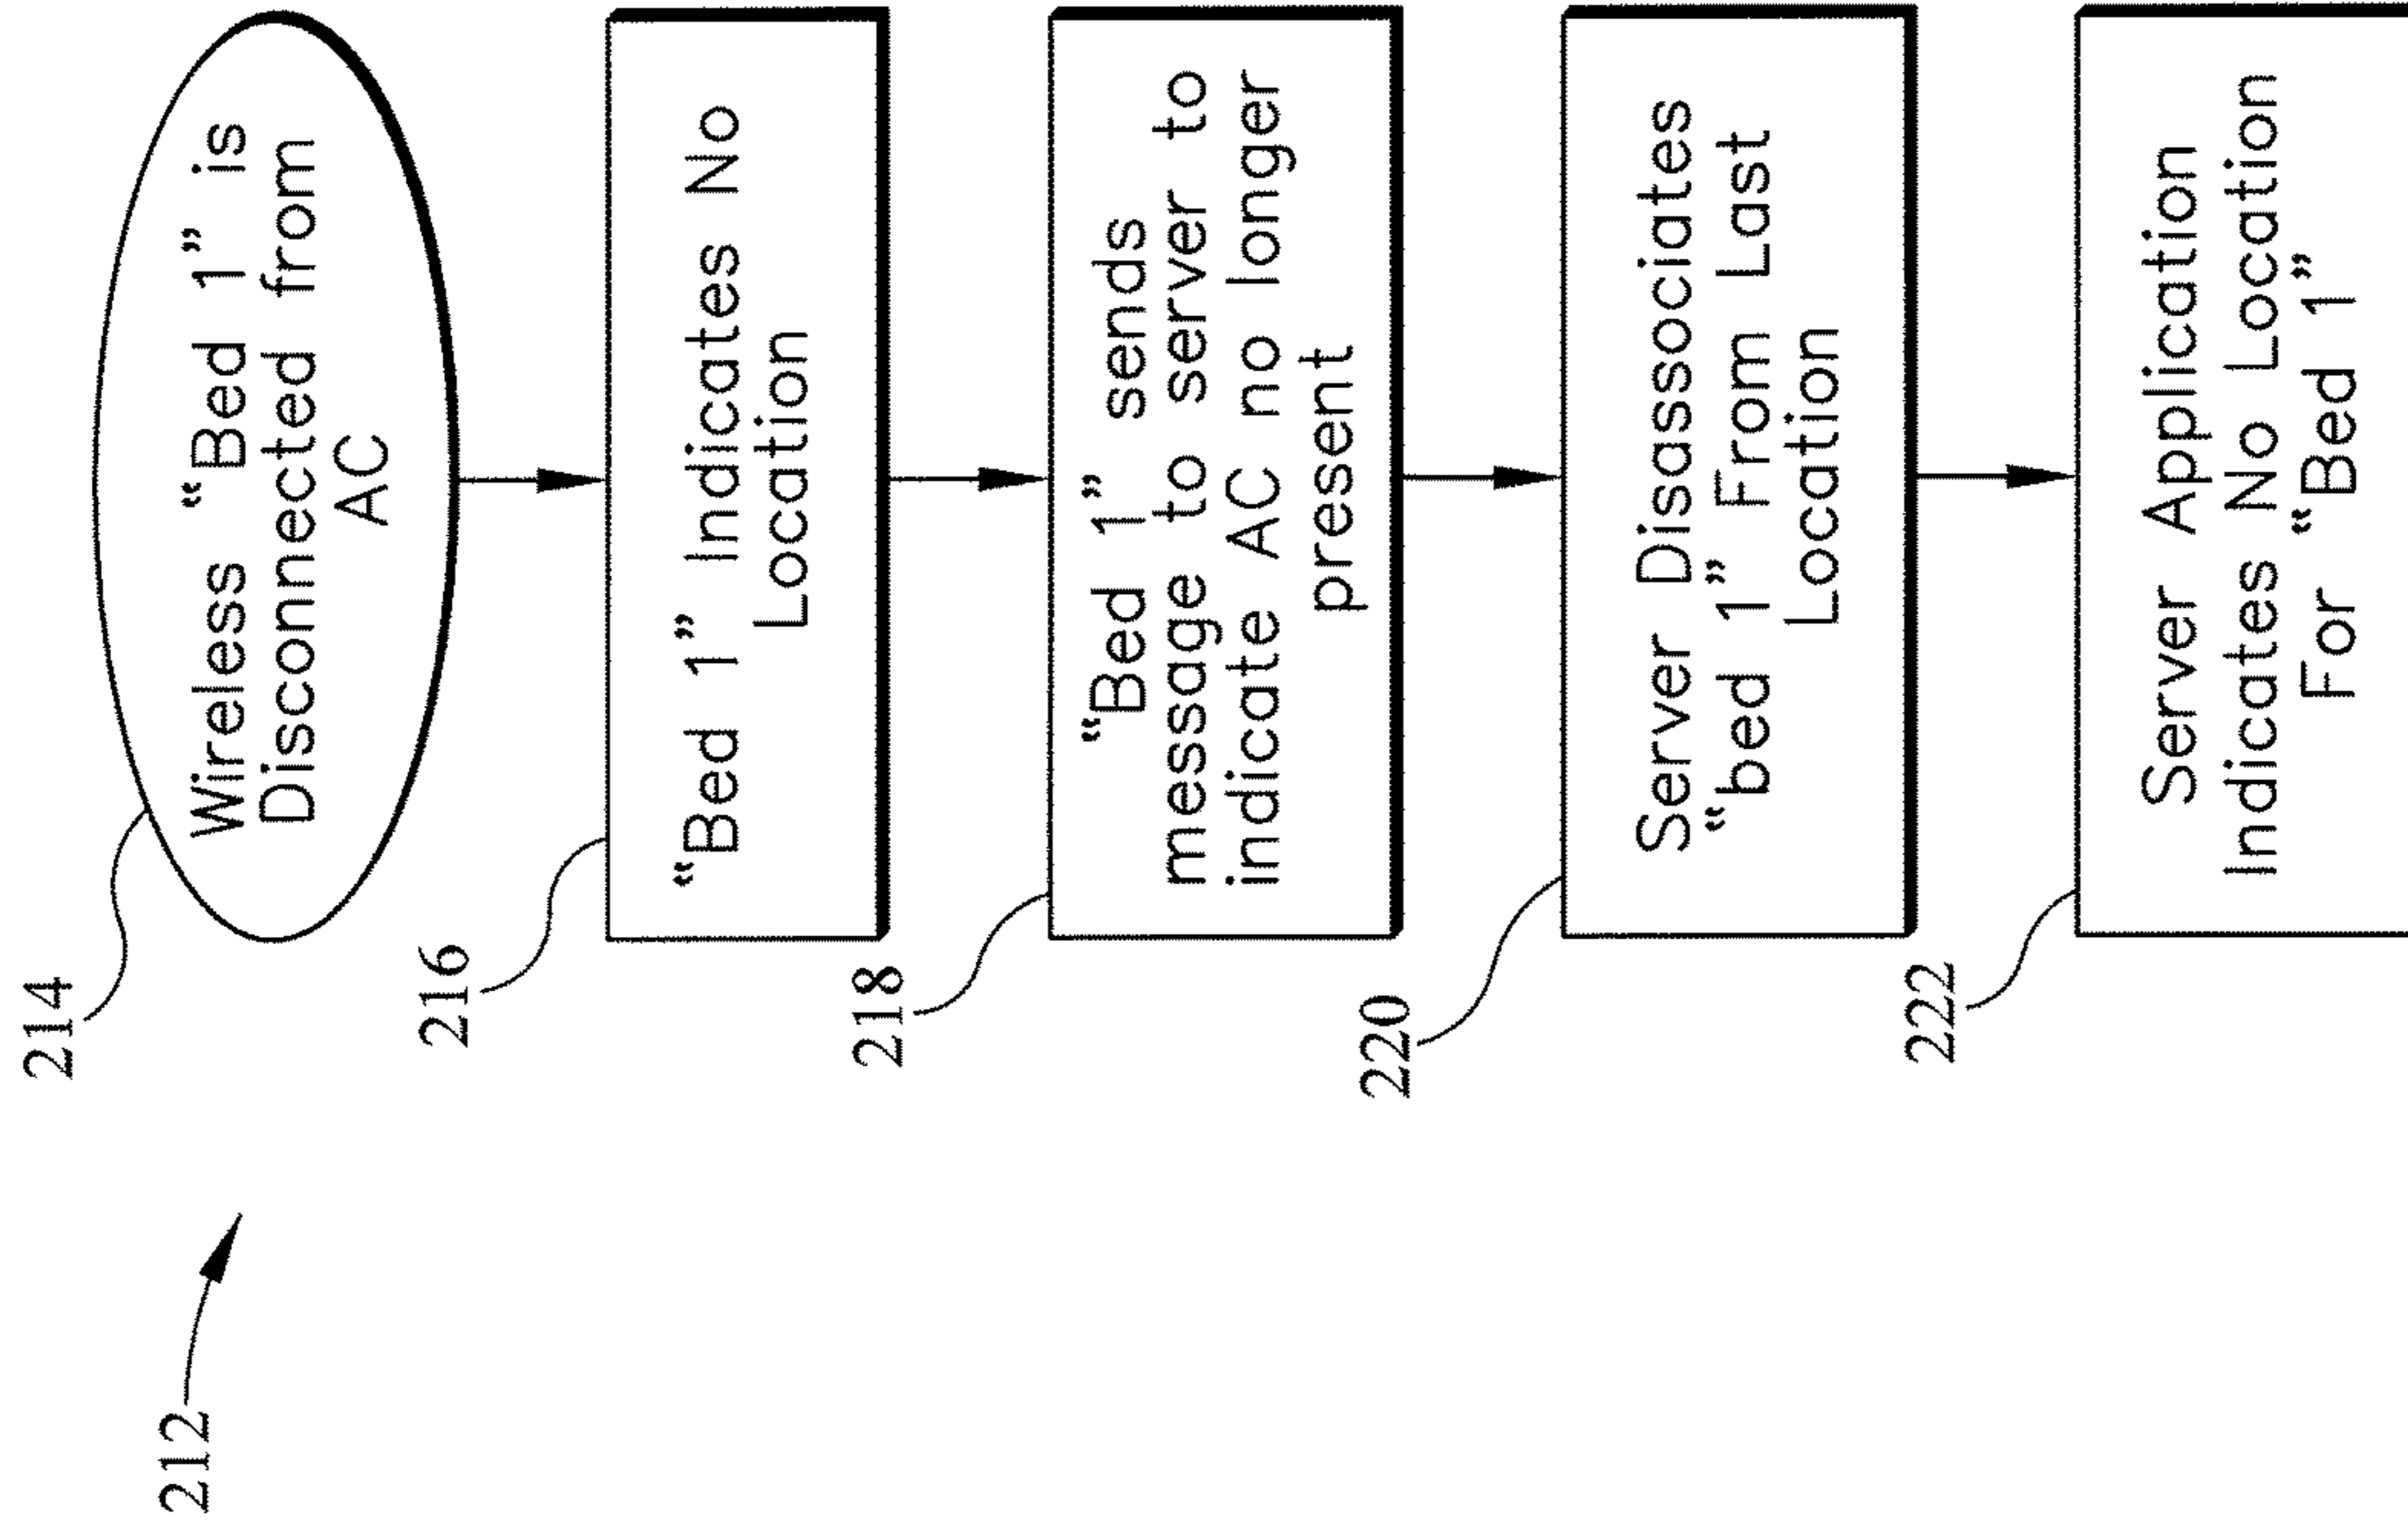


FIG. 18

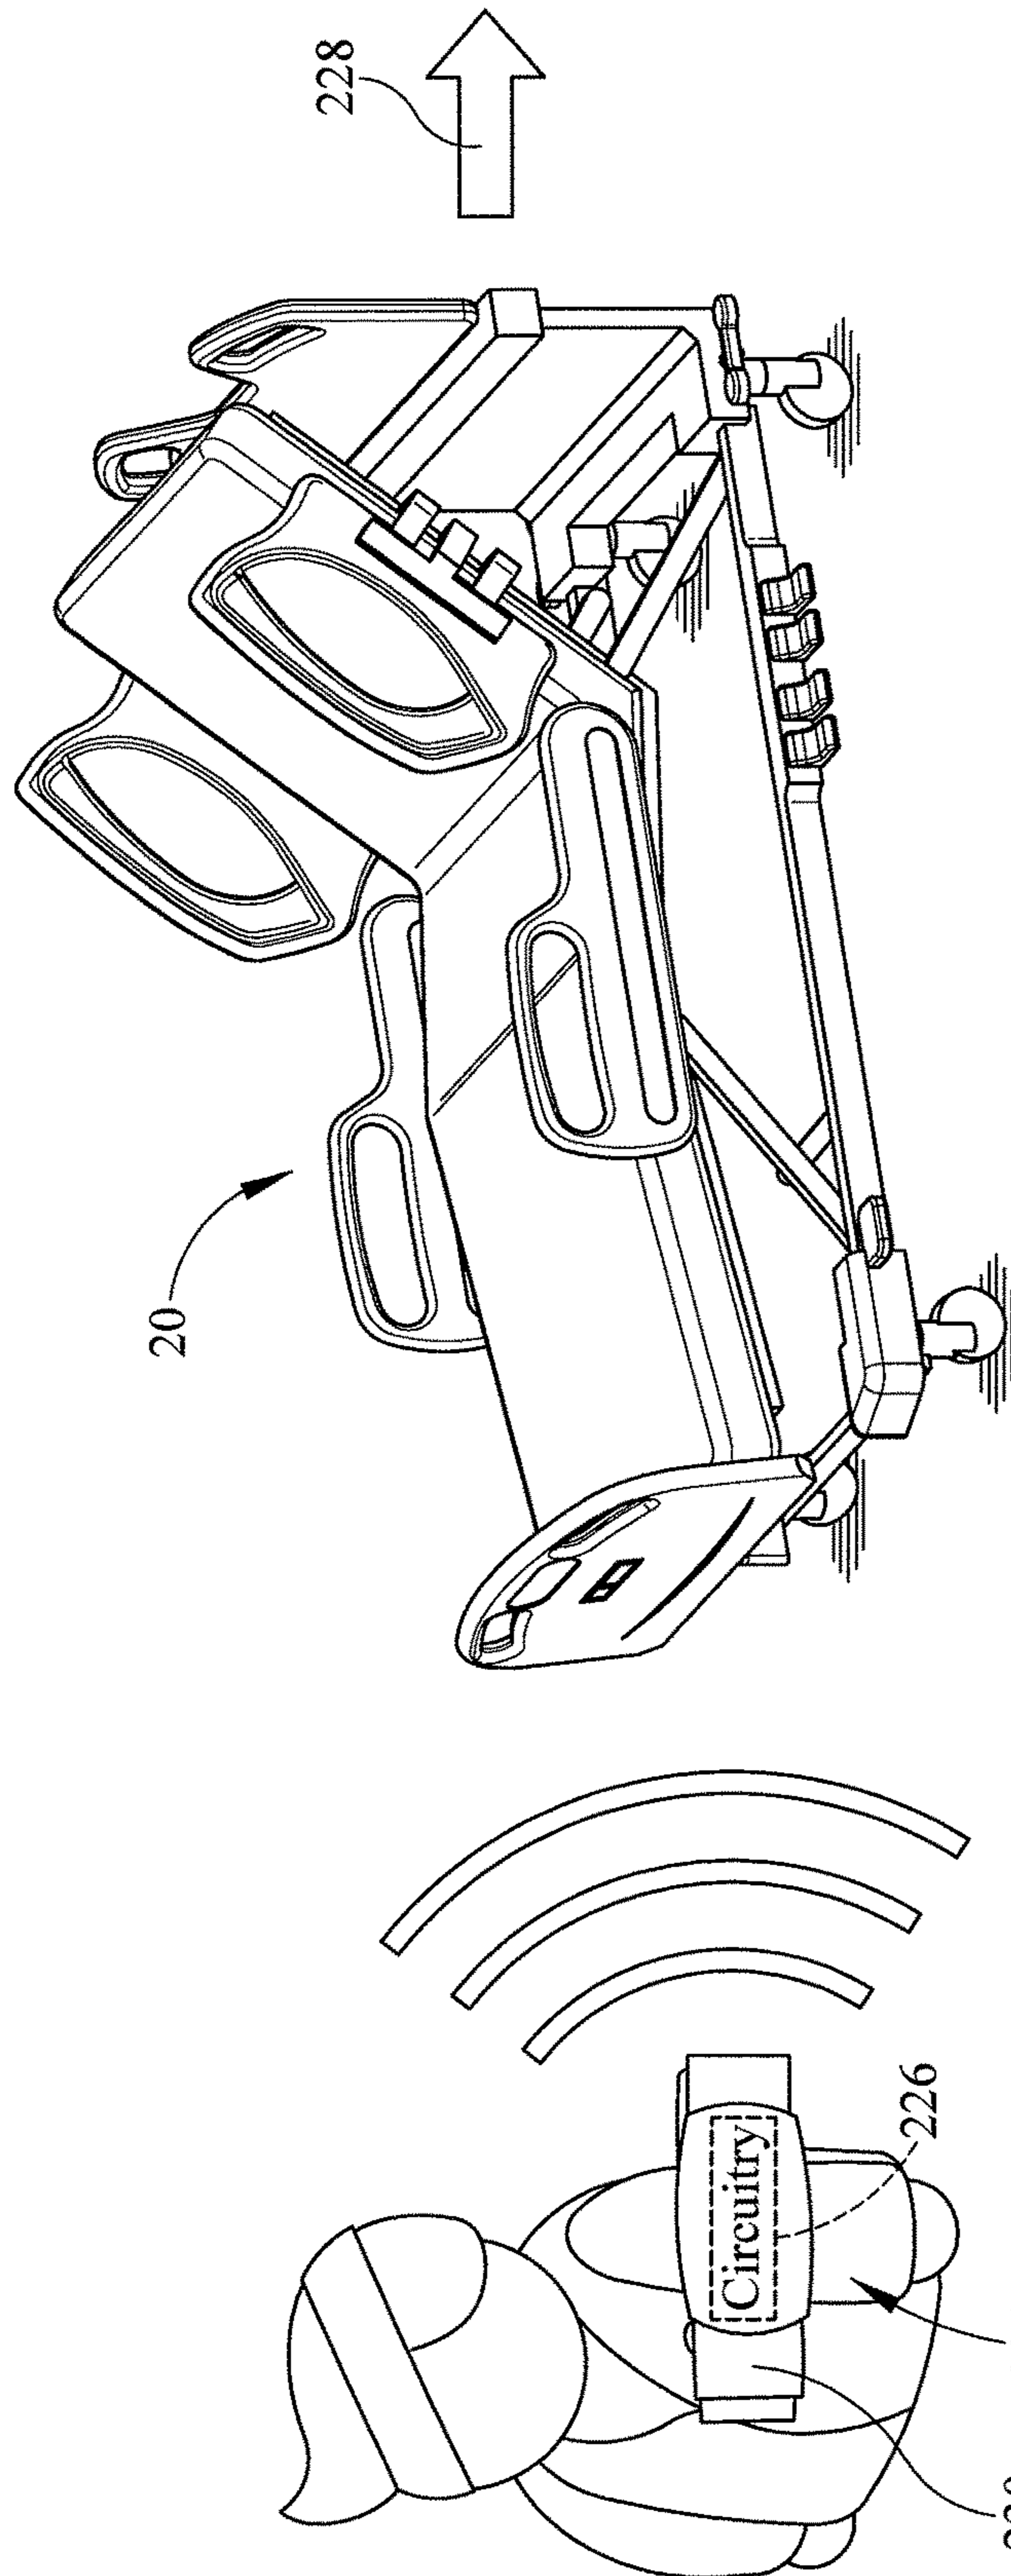


FIG. 19

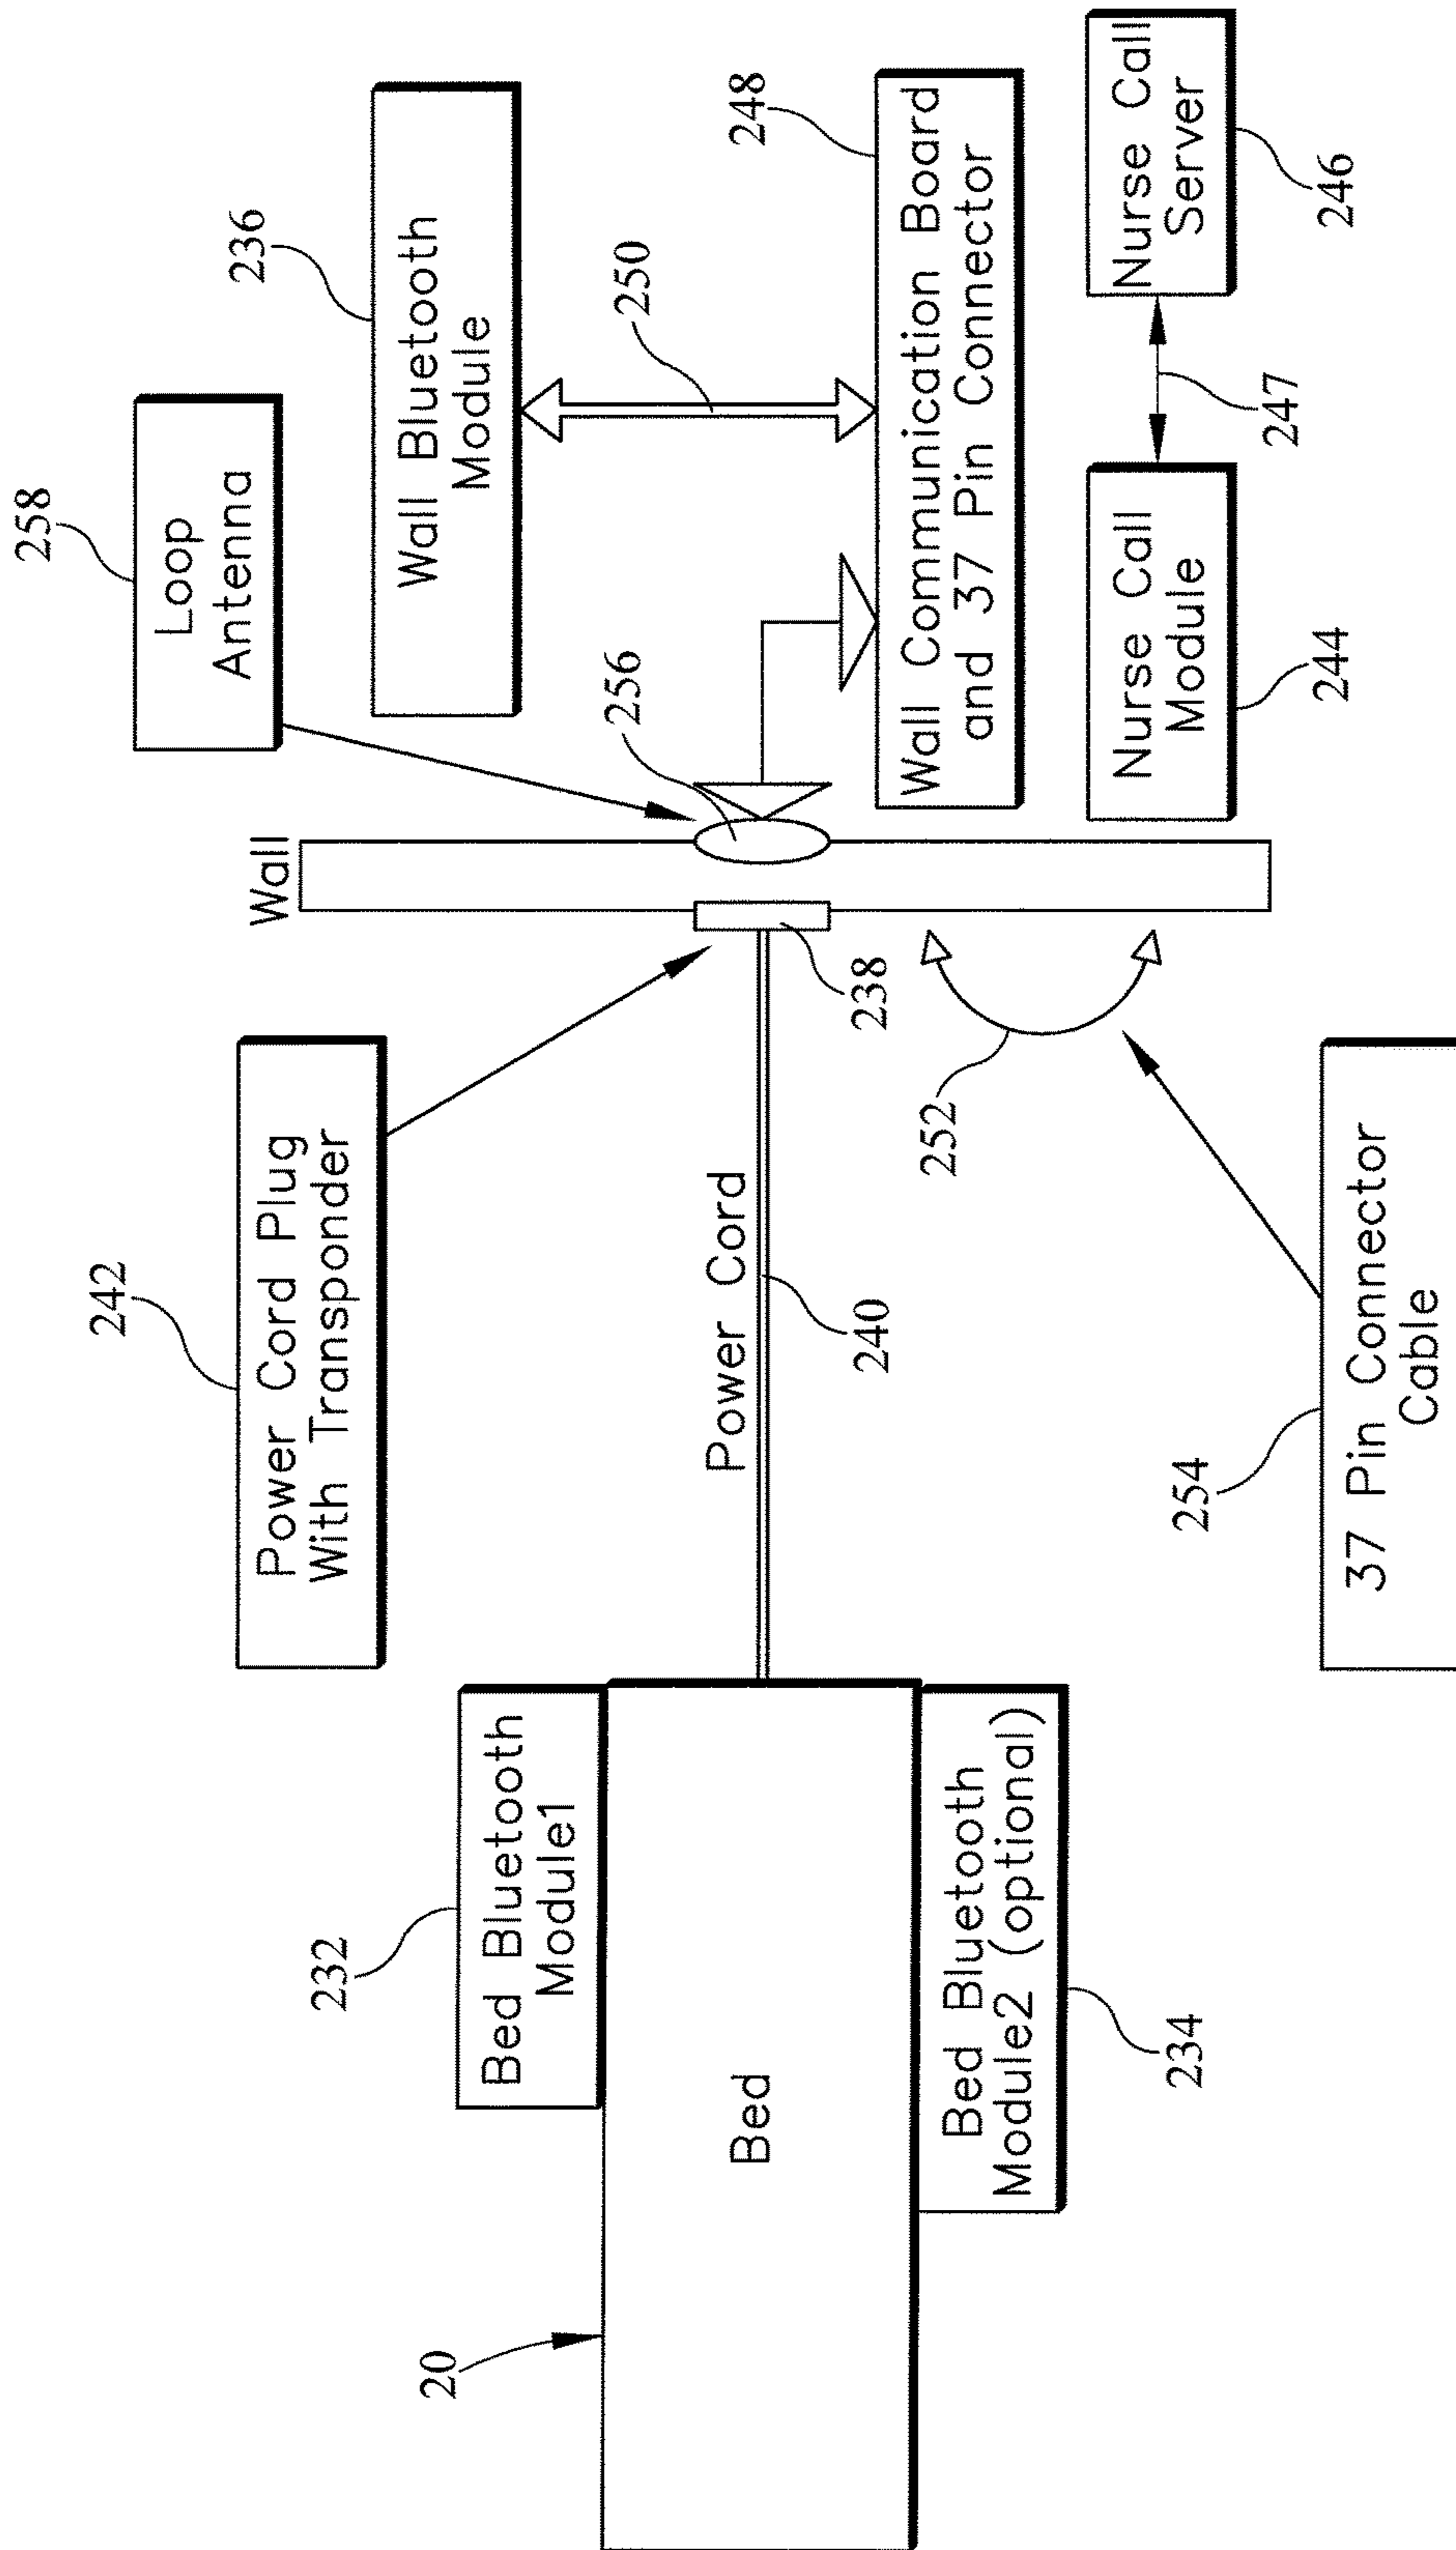


FIG. 20

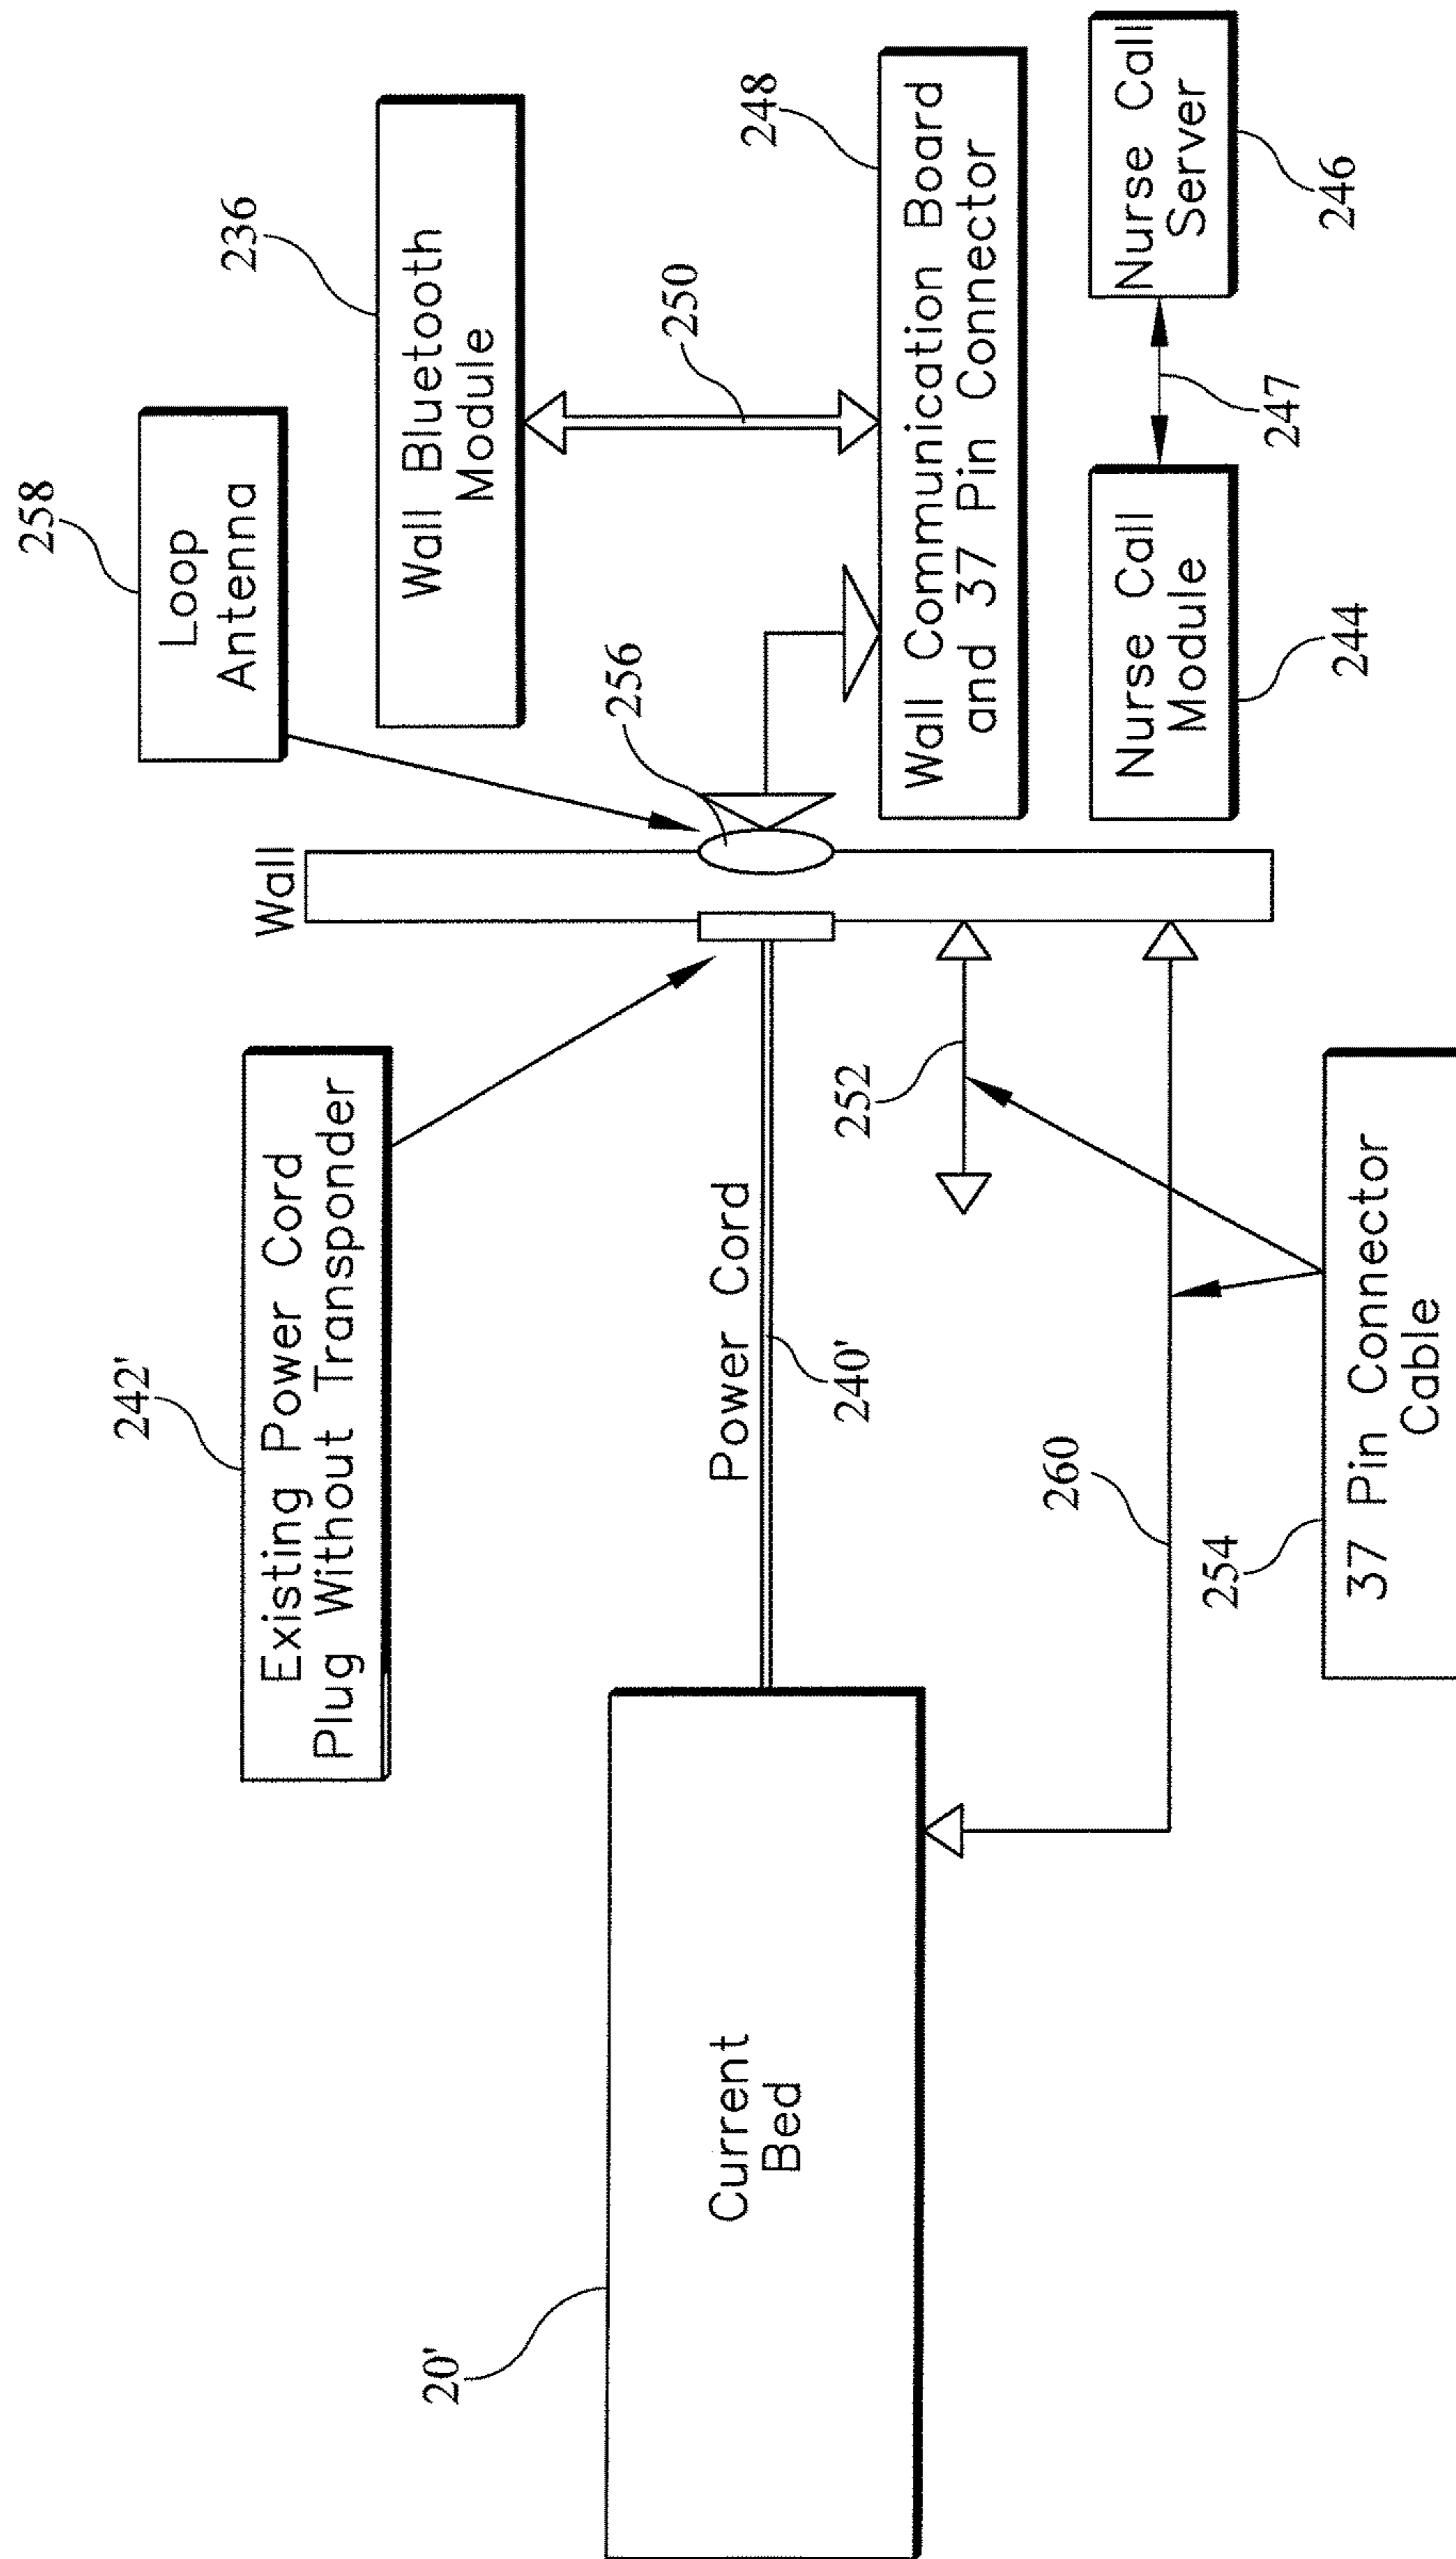


FIG. 21

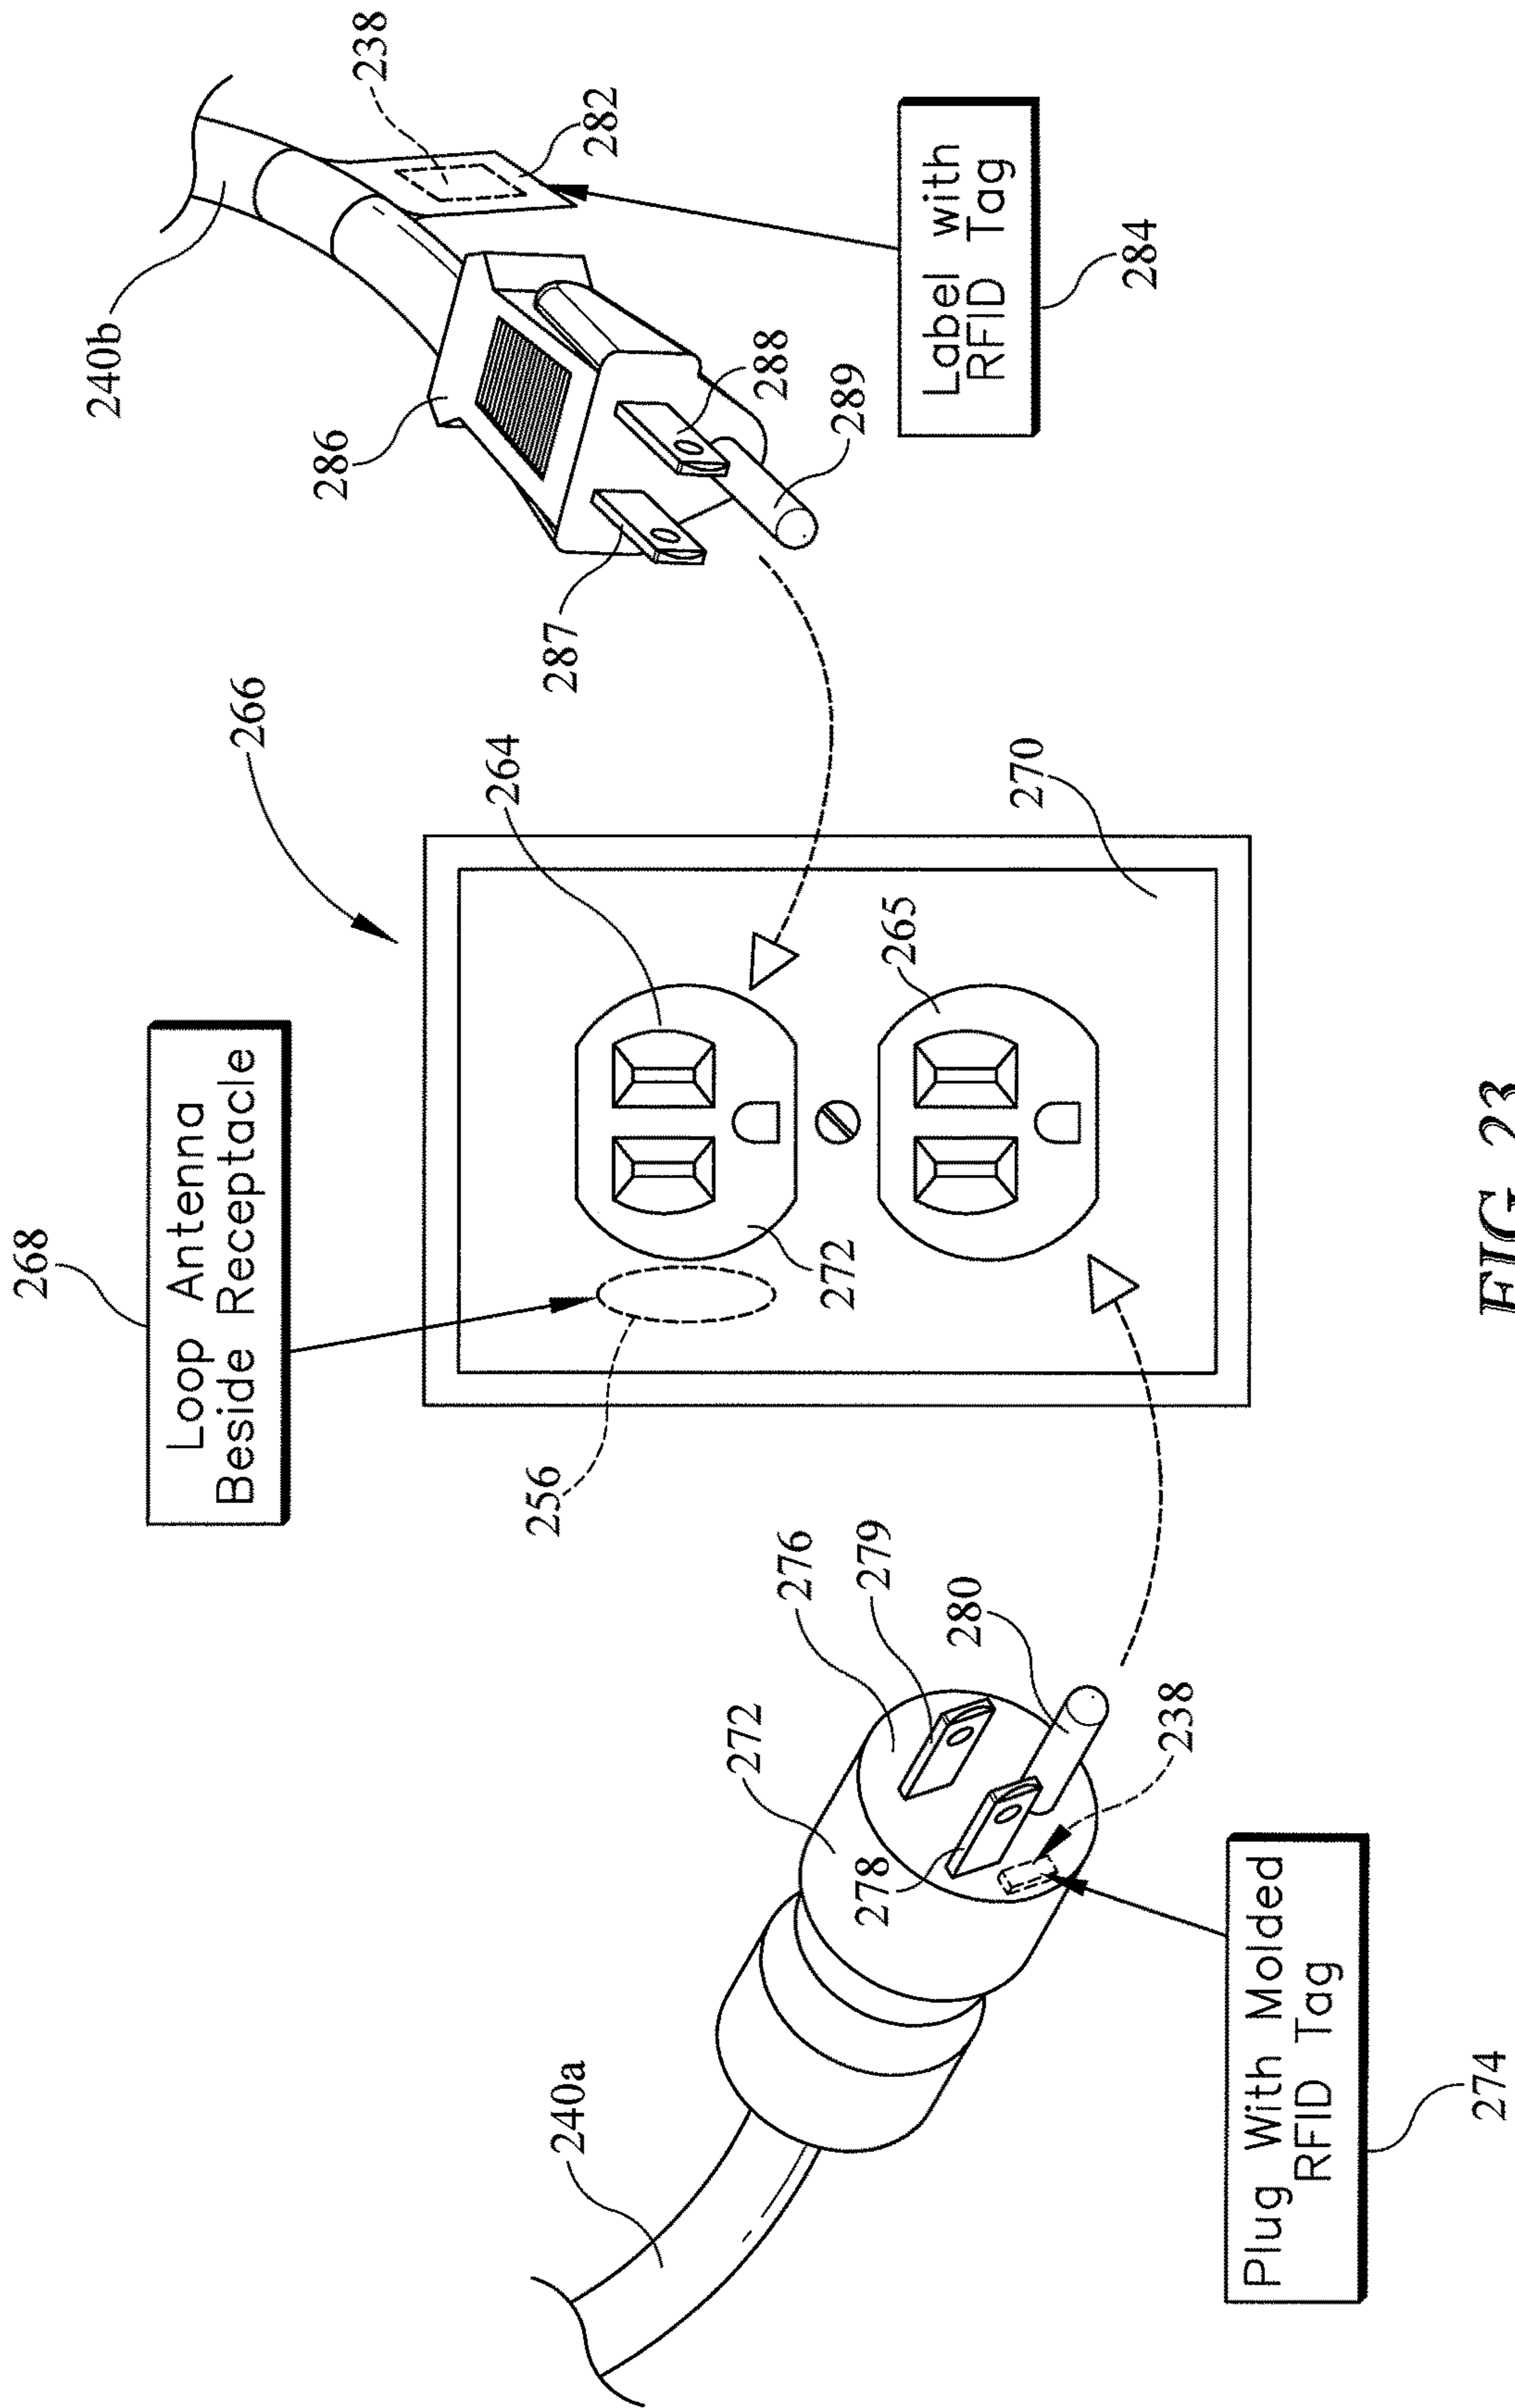


FIG. 23

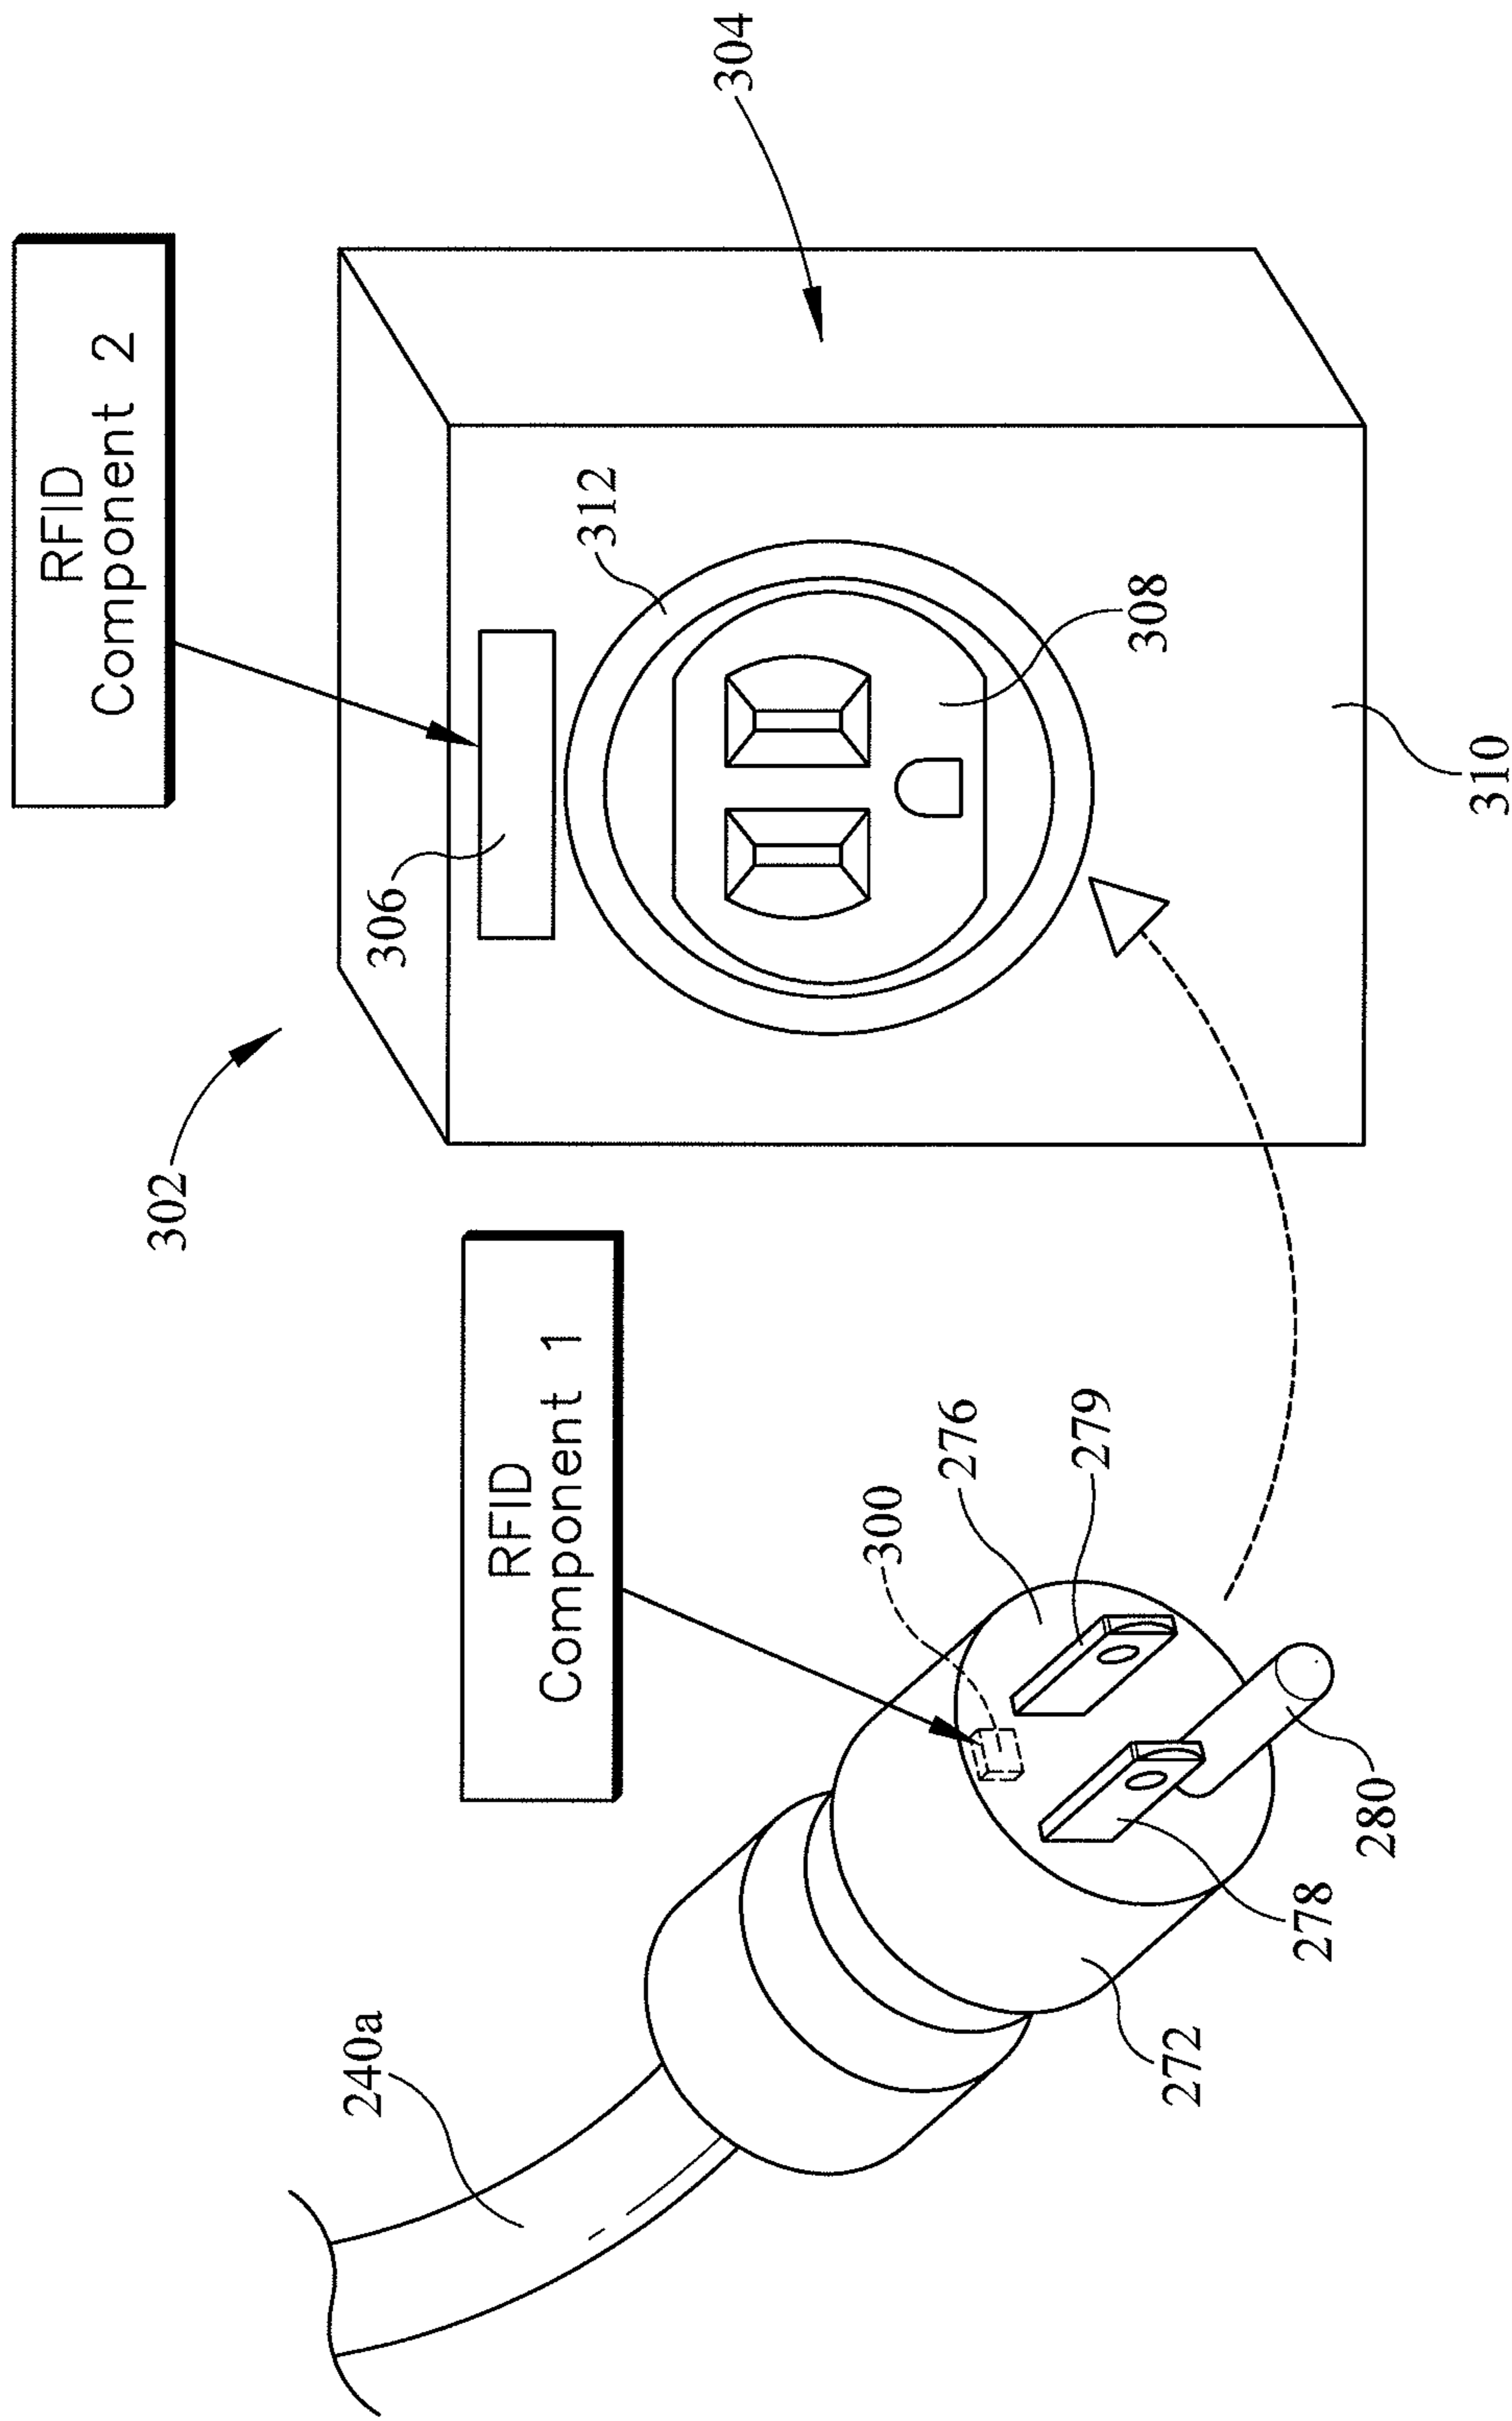


FIG. 24

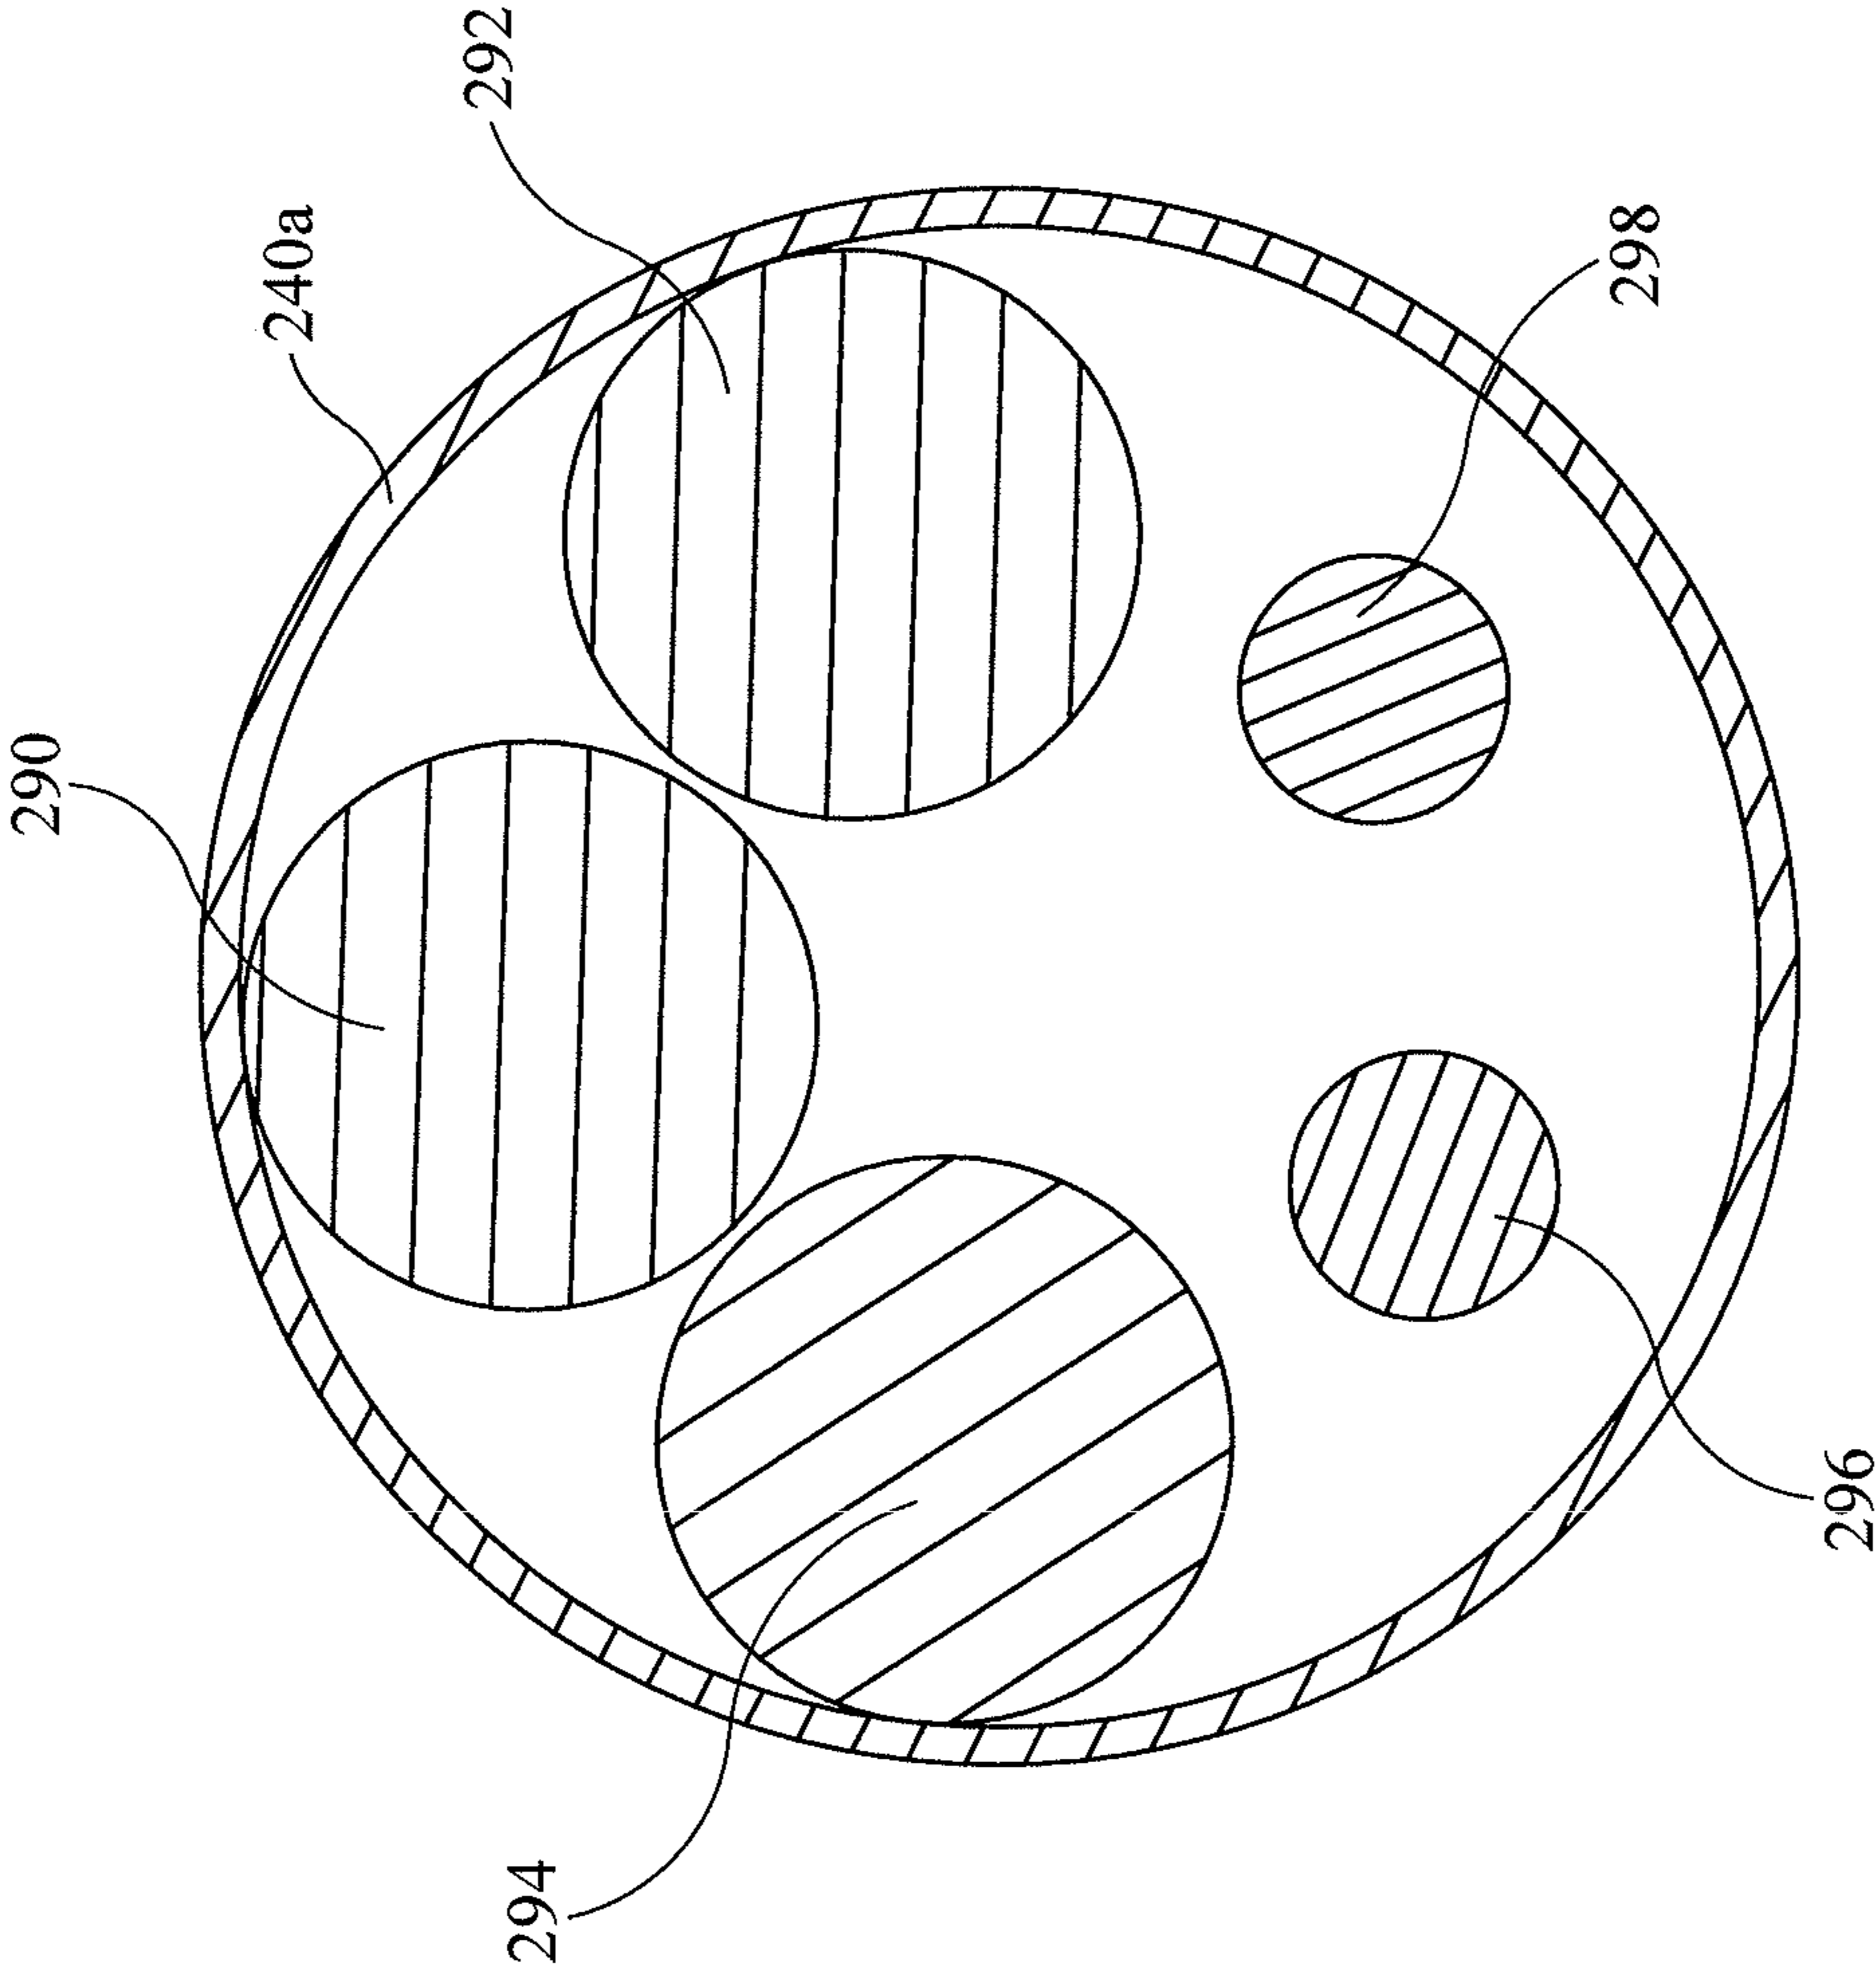


FIG. 25

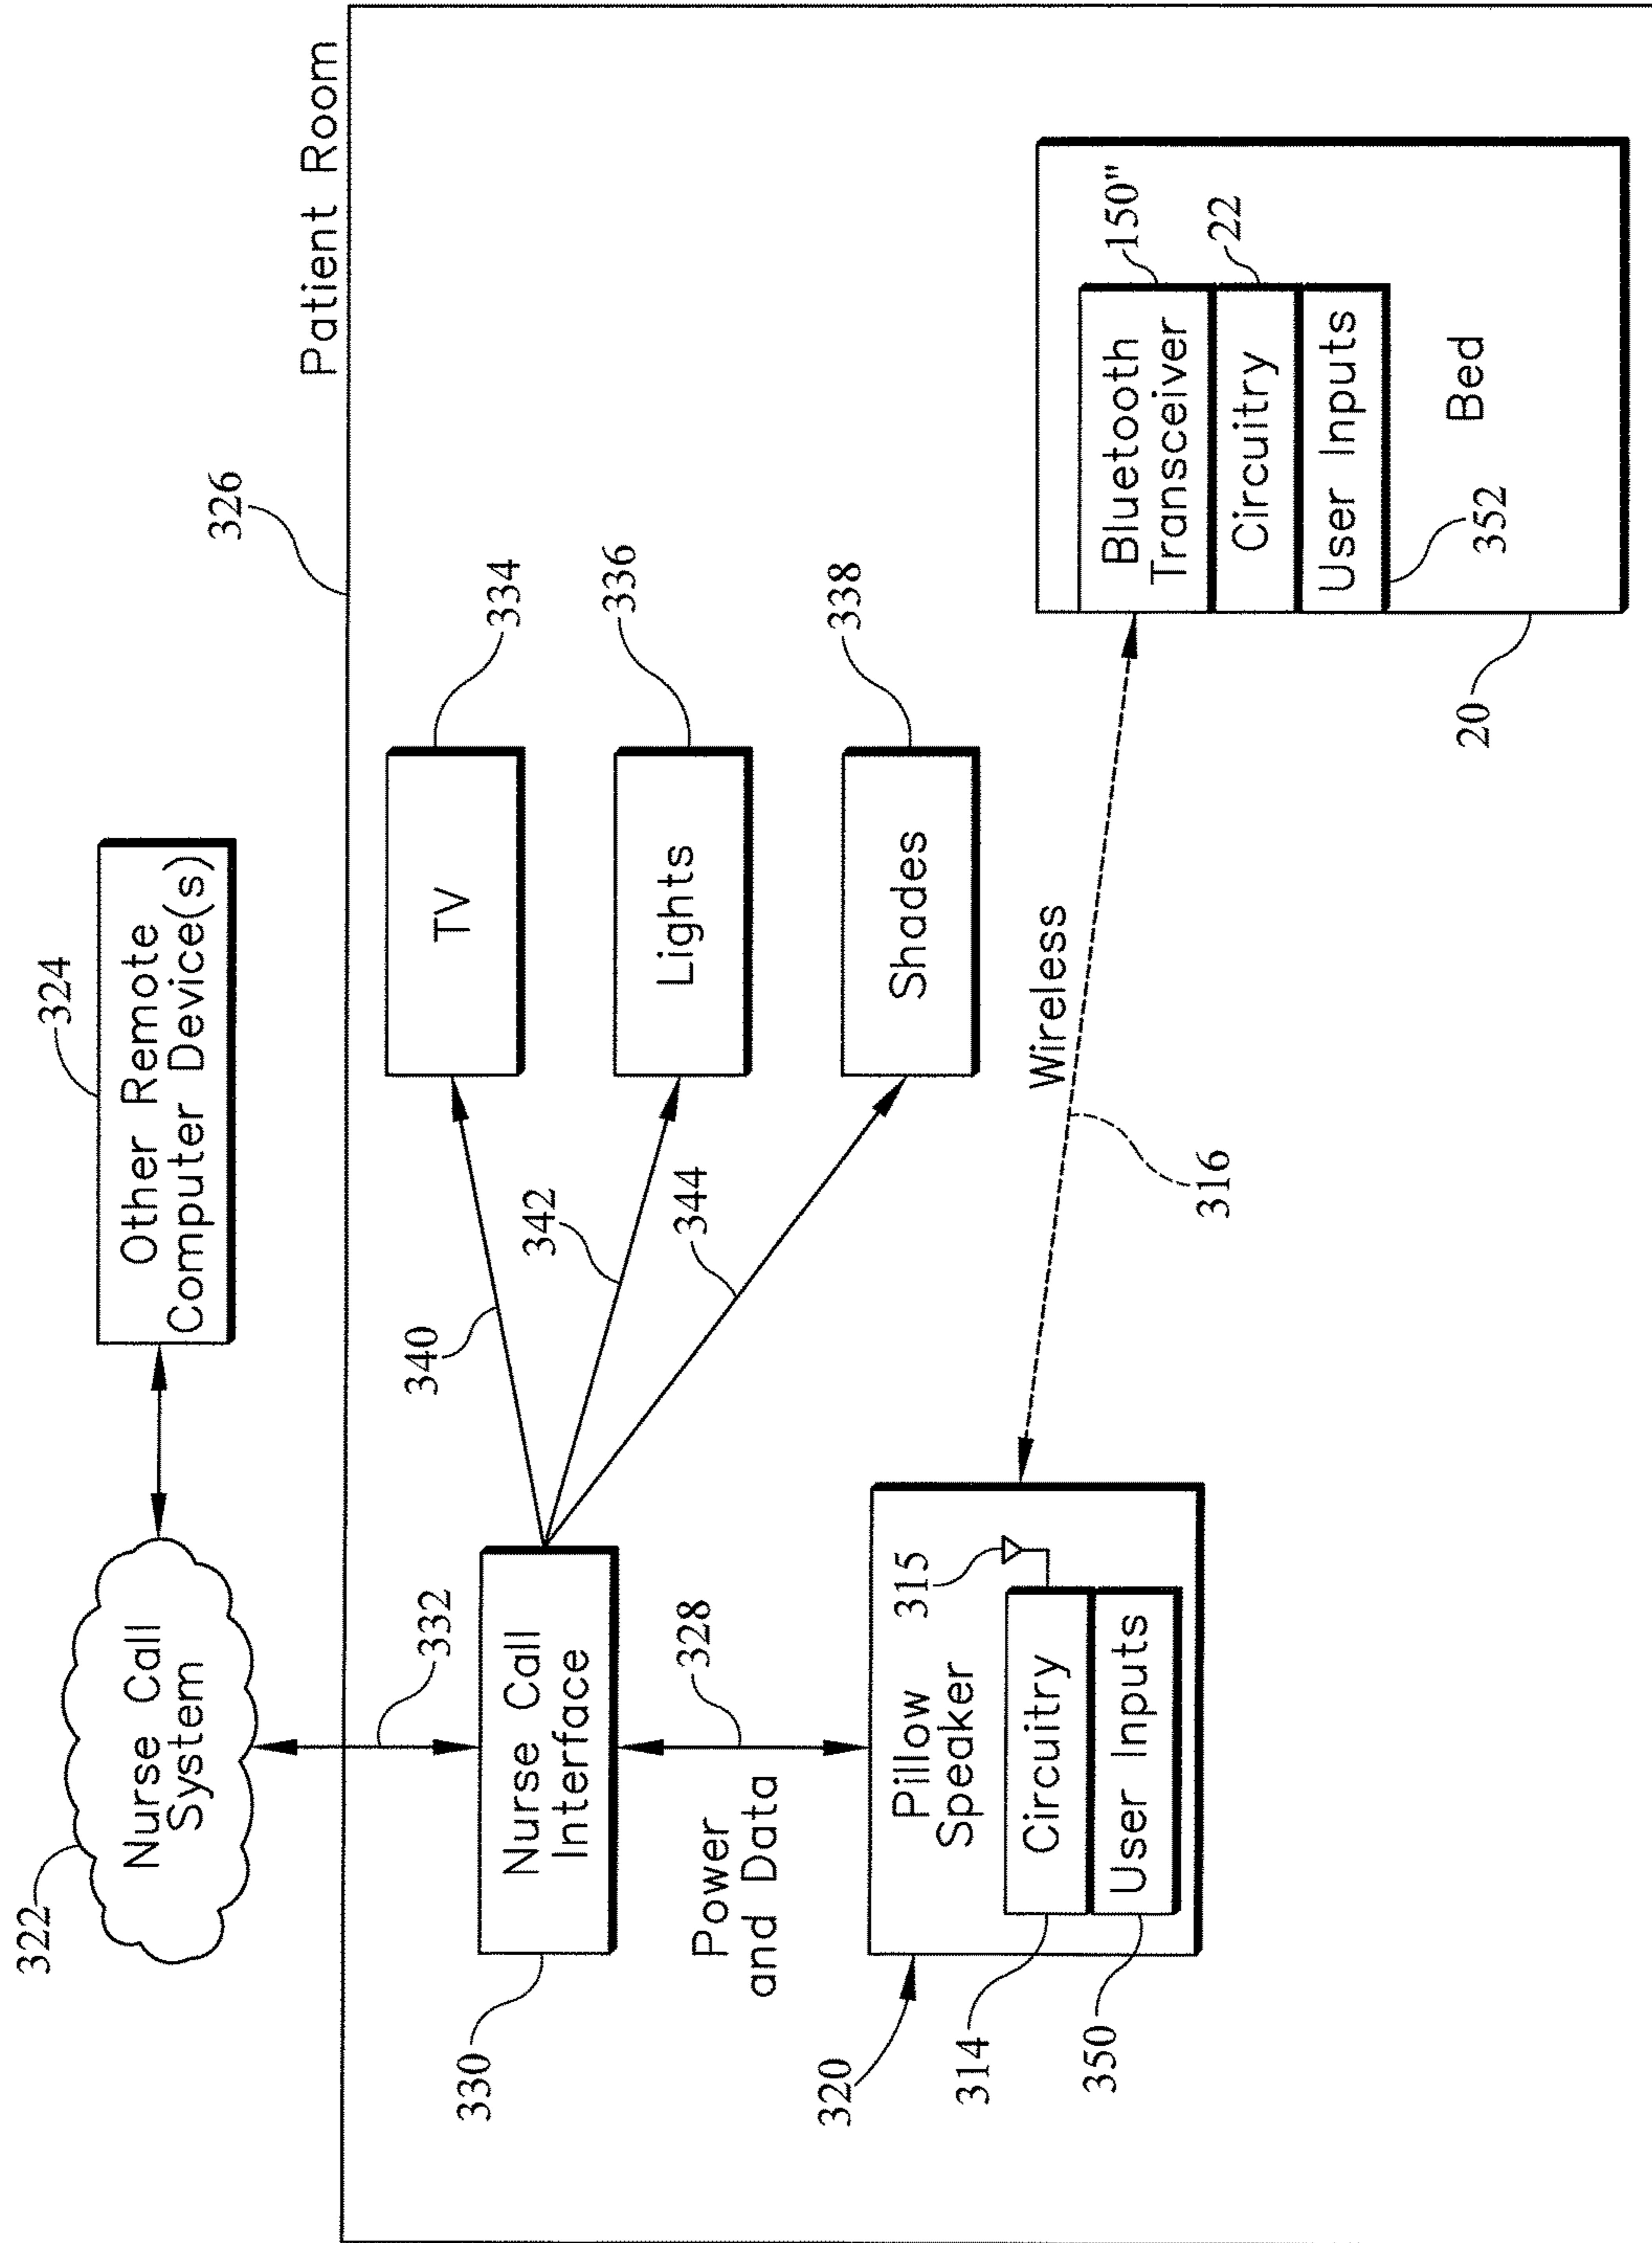
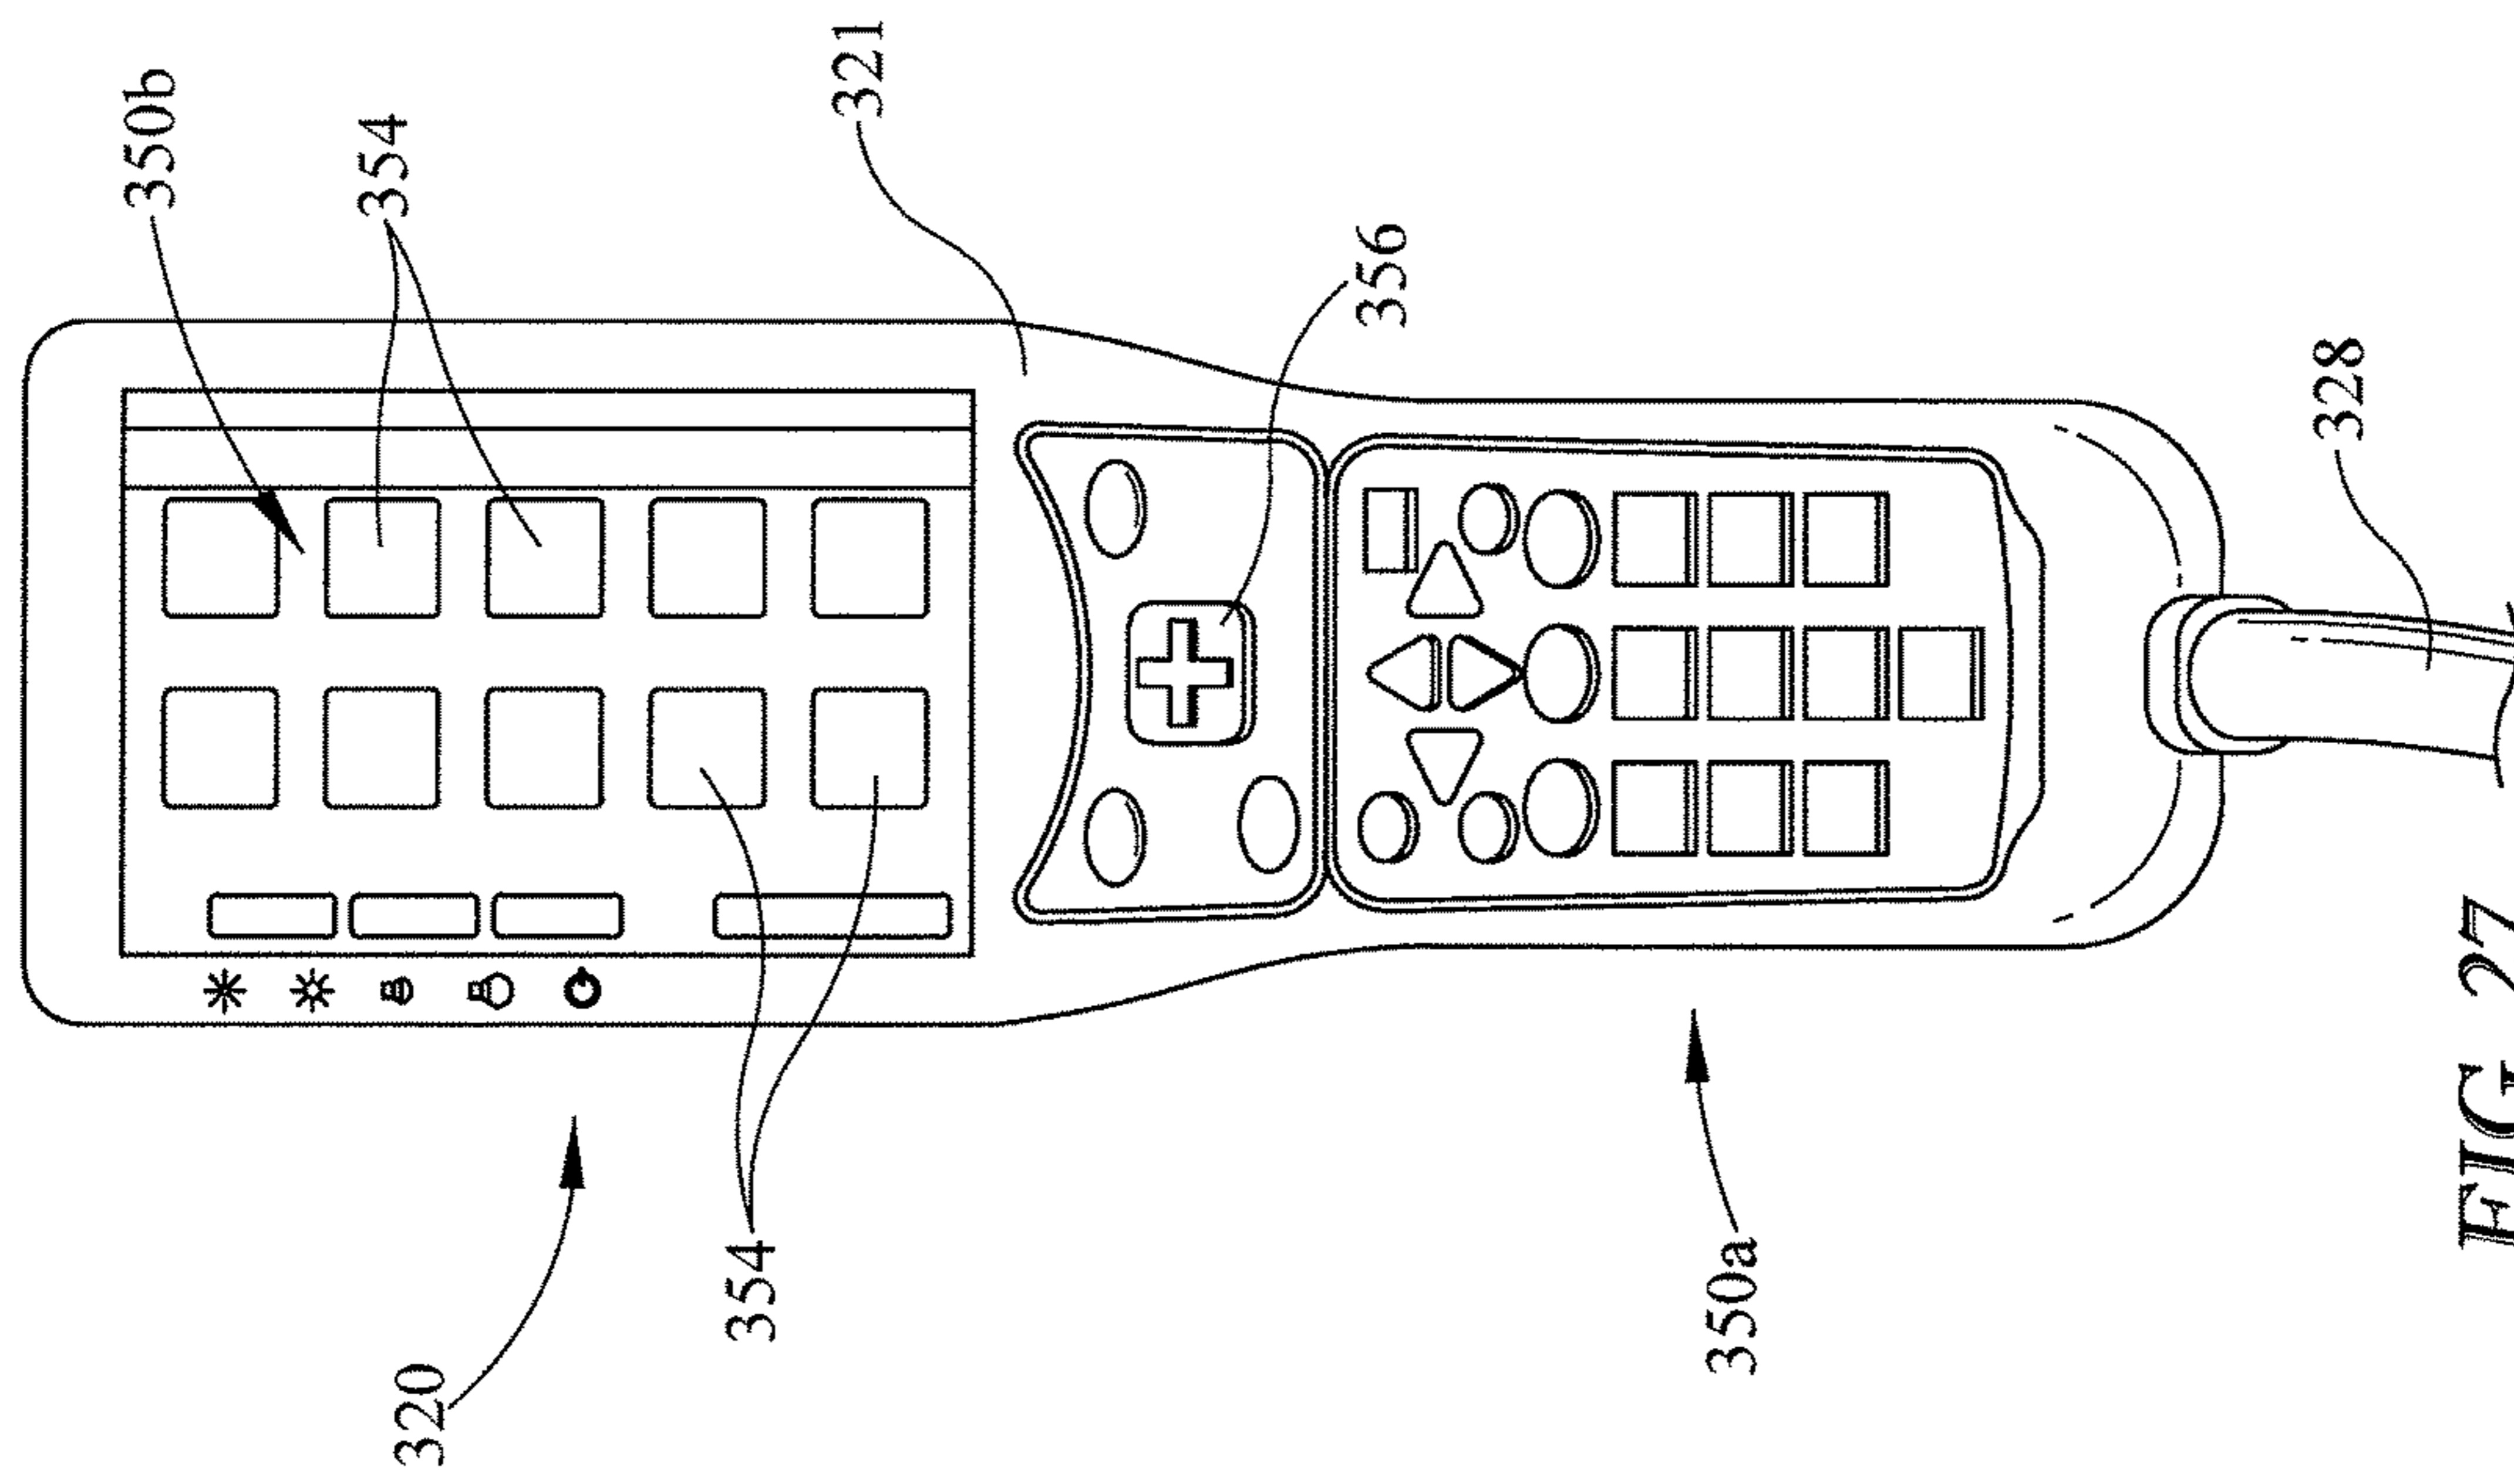


FIG. 26



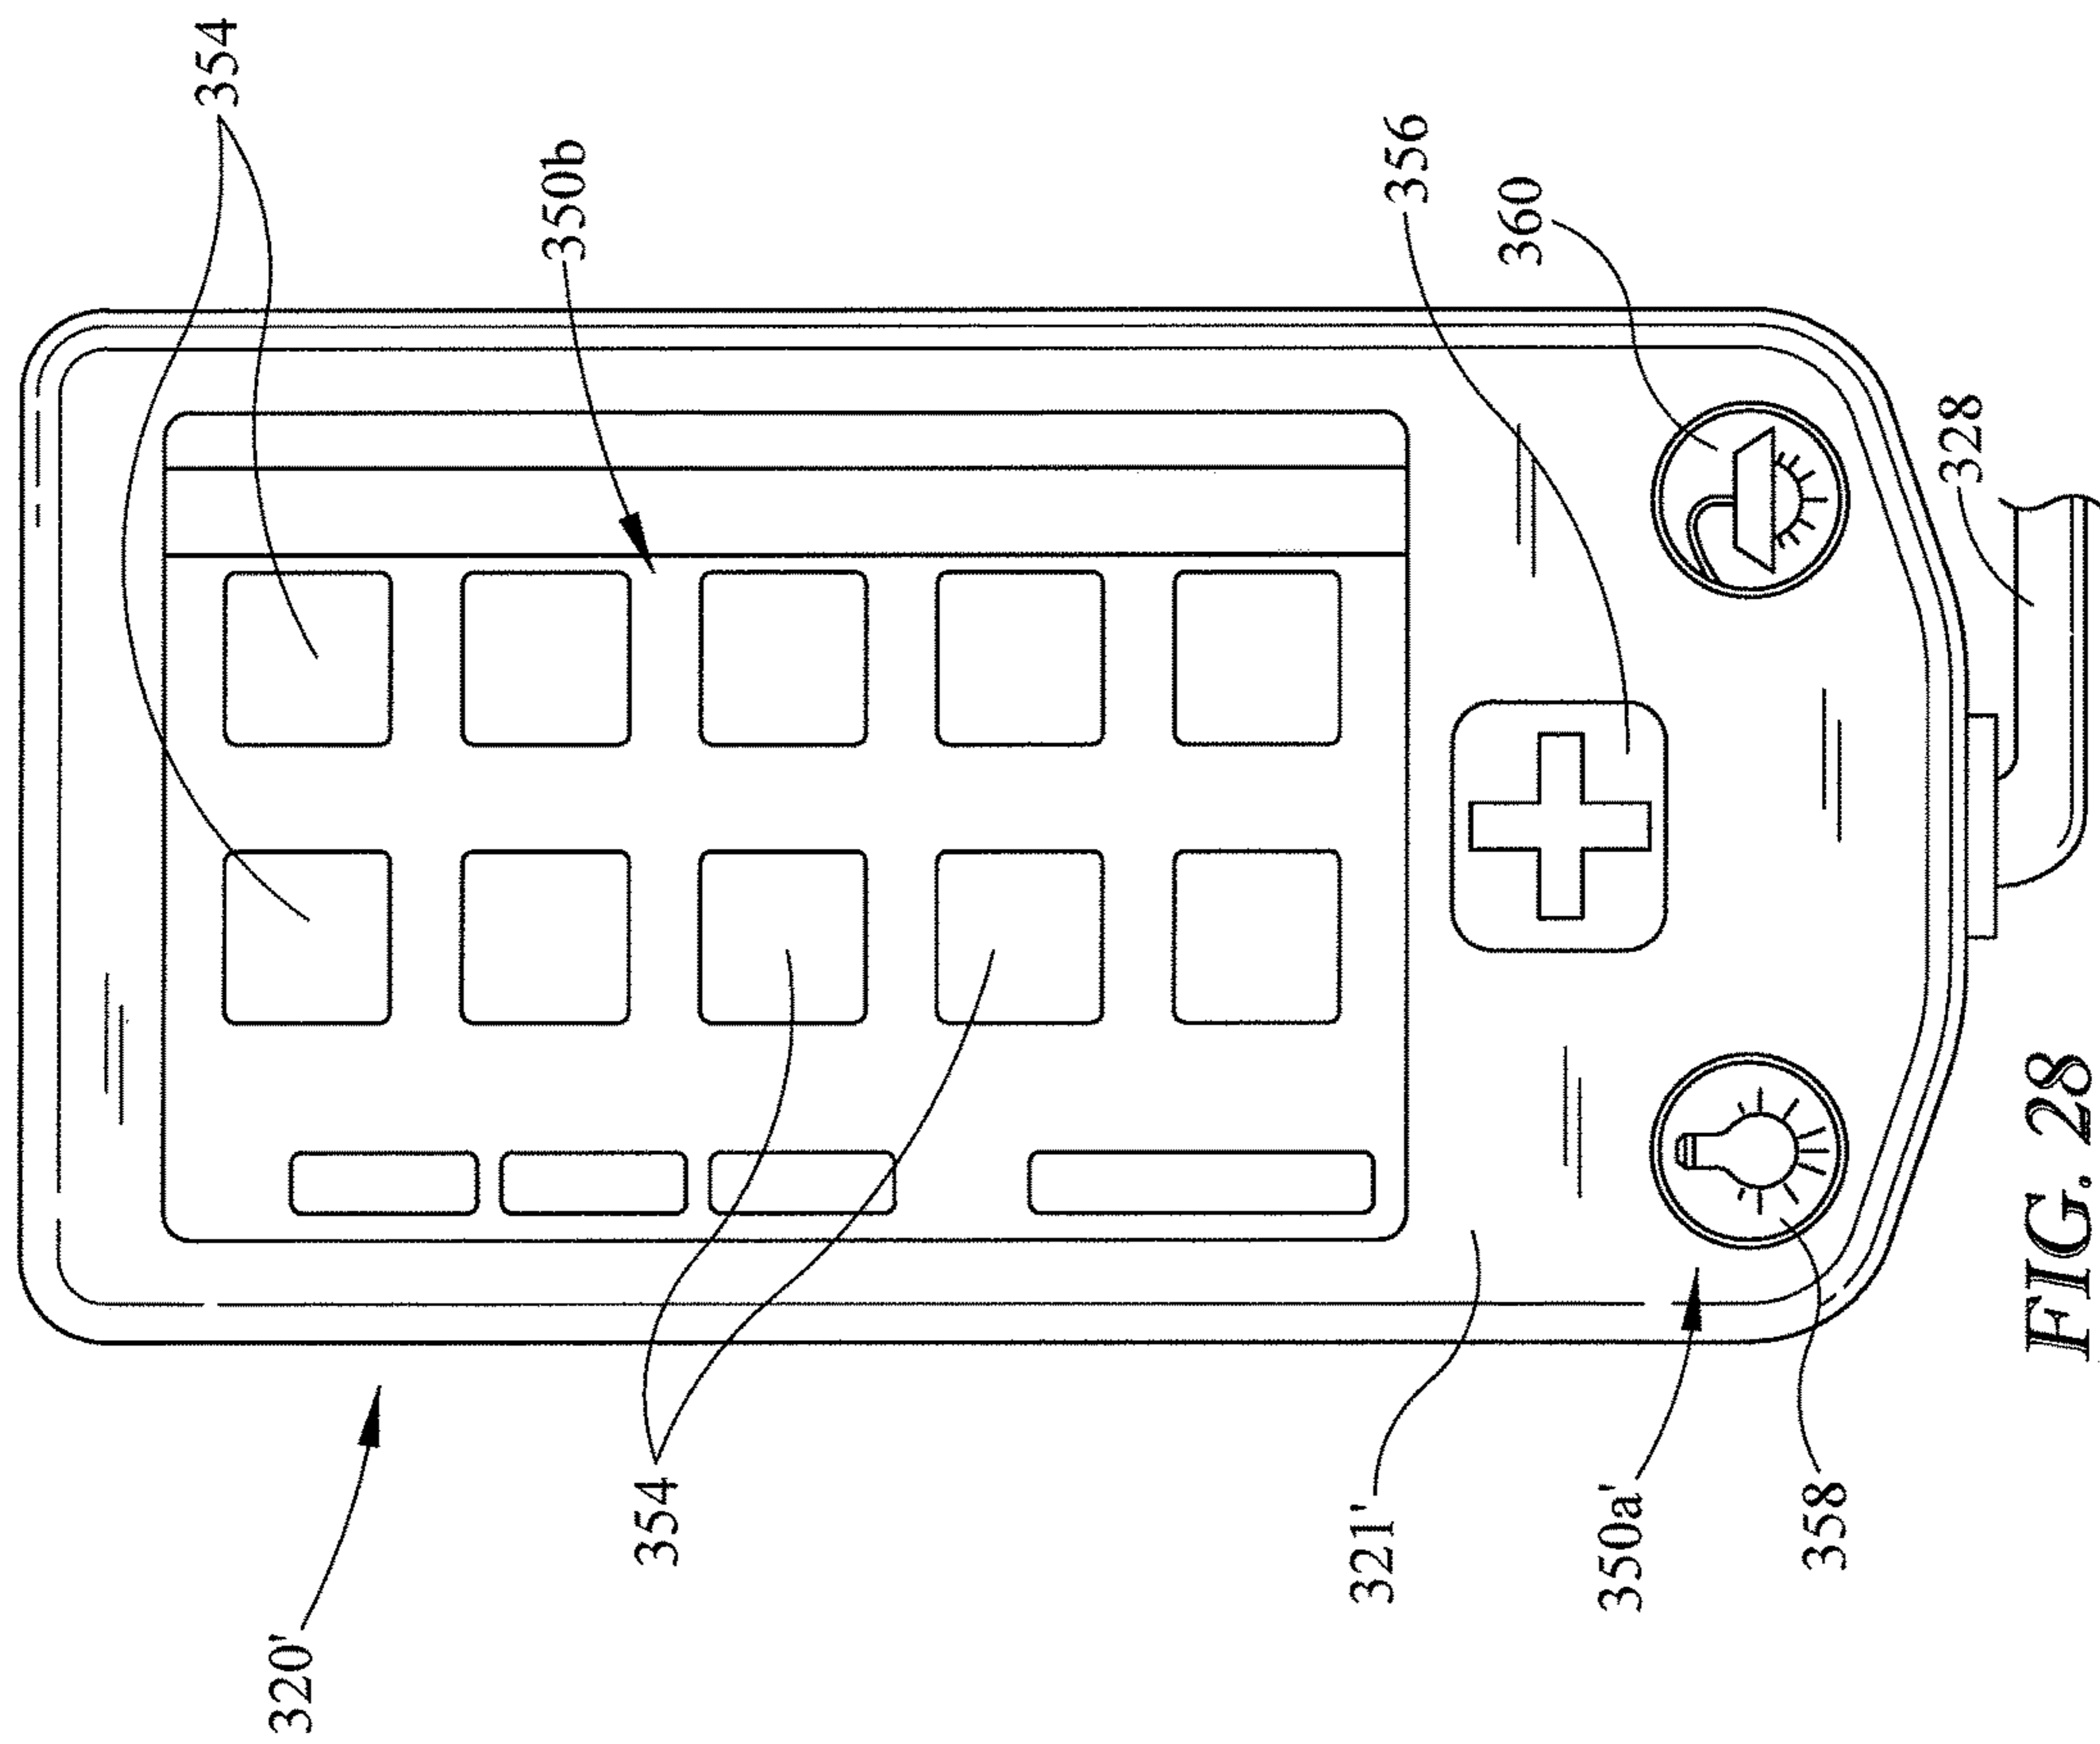


FIG. 28

BED/ROOM/PATIENT ASSOCIATION SYSTEMS AND METHODS

CROSS REFERENCE TO RELATED APPLICATIONS

The present application is a continuation of U.S. application Ser. No. 14/487,279, filed Sep. 16, 2014, now U.S. Pat. No. 9,830,424, which claims the benefit, under 35 U.S.C. § 119(e), of U.S. Provisional Application No. 61/879,399, filed Sep. 18, 2013, and each of which is hereby incorporated by reference herein in its entirety.

BACKGROUND

The present disclosure relates to systems and methods for associating beds, rooms, and/or patients and particularly, to such association systems and methods used in a healthcare facility.

Systems and methods for determining the location of a patient bed within a healthcare facility are known. In some of the known systems, a locating tag is attached to the bed and periodically transmits a wireless signal that includes a tag identifier (aka a "tag ID") which is a string of characters such as letters and/or numbers and/or symbols that uniquely identify the tag. In some such prior art systems, a set of wireless receivers are mounted at fixed locations throughout the healthcare facility and are coupled to the computer network of the healthcare facility. A receiver in the vicinity of a tag receives the tag ID and transmits it along with a receiver ID to other computer devices of the network. Each receiver ID corresponds to a location in the healthcare facility. Thus, one or more remote computer devices are able to determine the location of the bed based on the tag ID and the receiver ID.

In many of the prior art systems, the wireless signal from the tag is an infrared signal that requires an uninterrupted line of sight to a receiver. If the line of sight is blocked, the receiver does not receive the signal from the tag. Thus, in more recent times, the desire has been to use radio frequency (RF) tags but the drawback with those systems is that RF signals are able to penetrate floors, ceilings and walls in a healthcare facility such that multiple receivers sometimes receive the same wireless RF signal and further processing of some type is needed to resolve the ambiguity of the bed's location. Some prior art systems have resolved the ambiguities by analyzing signal strength or analyzing time of flight information.

In some known prior art systems, patient beds have circuitry that transmits a bed ID, as opposed to a tag ID, as well as bed status data from the beds. Typically, the transmissions are made over a cable that extends from the bed to some sort of interface unit mounted to a wall in a room, but there is the option to do this wirelessly in some prior art systems by using a wireless interface unit mounted to the room wall. In any event, the interface unit that receives the transmissions from the bed, either via a wired or wireless connection, is then connected to the network of the healthcare facility, typically, via a wired connection. In these prior art systems, the installation of interface units just to receive bed ID and bed status data is an added cost to the overall network of the healthcare facility.

The use of wireless access points in healthcare facilities to receive Wi-Fi signals from a variety of equipment and computer devices is becoming more widespread. Thus, there is a need to develop systems and methods for making bed-to-room associations or patient-to-room associations or

patient-to-bed associations or patient-to-bed-to-room associations that minimize the amount of specialized receivers, interface units, or other equipment that must be coupled to the network of the facility.

SUMMARY

The present invention may comprise one or more of the features recited in the appended claims and/or the following features which each are considered to be optional and which, alone or in any combination, may comprise patentable subject matter:

A system for use in a healthcare facility that may have a network may be provided according to this disclosure. The system may include a light source that may emit visible light that may have a signature that may be unique to a location of the healthcare facility. The system may also include a patient bed that may have circuitry that may analyze the light from the light source to determine the signature corresponding to the location. The circuitry may be configured to transmit data corresponding to the signature and to transmit bed identifier (ID) to the network.

In some embodiments, the signature may comprise a specified wavelength. The light source may be programmable to emit light at the specified wavelength. Alternatively or additionally, the signature may comprise a specified pulse frequency that may be sufficiently great so as to be imperceptible by human vision. The light source may be programmable to emit light at the specified pulse frequency. Thus, the signature may comprise a specified wavelength at a specified pulse frequency in some embodiments. In such embodiments, the light source may be programmable to emit light at the specified wavelength and at the specified pulse frequency.

According to this disclosure, the light source may comprise a light bulb that provides room lighting. In other embodiment, the light source may comprise a display screen, such as one that may be mounted to a ceiling or a wall of a room of the healthcare facility. The display screen may be the display screen of a computer device such as the display screen of a room station of a nurse call system, for example. There may be a light source in a number of rooms and the signature from the light source, be it a light bulb or a display screen, may be different for each room. The light source may include at least one light emitting diode (LED).

Further according to this disclosure, the circuitry of the patient bed may include a red-green-blue image sensor that may sense the light emitted by the light source. Alternatively or additionally, the circuitry of the patient bed may include a camera that receives the light emitted by the light source.

The system may further include a computer device that may be coupled to the network remote from the light source and the patient bed. The computer device may determine the location of the healthcare facility in which the light source may be located based on the data corresponding to the signature. The computer device may associate the bed ID with the location of the healthcare facility.

In some embodiments, the circuitry of the patient bed may wirelessly transmits the data corresponding to the signature and the bed ID to the computer device via a wireless access point of the network. Alternatively or additionally, the circuitry of the patient bed may transmit the data corresponding to the signature and the bed ID to the computer device via a wired connection from the bed to the network.

According to some embodiments, a light source may emit visible light and infrared (IR) light. The IR light may have a signature that may be unique to a location of the healthcare

facility. A patient bed may include circuitry that may analyze the IR light from the light source to determine the signature corresponding to the location. The circuitry may be configured to transmit data corresponding to the signature and to transmit bed identifier (ID) to the network.

In some embodiments, the IR light may only be emitted when the visible light is turned off. According to this disclosure, the light source may include an energy storage device that may power the IR light while the visible light is turned off. The energy storage device may be charged when the visible light is turned on.

In some embodiments, the visible light may also be emitted with the signature such that the visible light and the IR light have the same signature. For example, the signature may comprise a specified pulse frequency. The specified pulse frequency may be programmable.

Further according to this disclosure, another system for use in a healthcare facility having a network may be provided. The system may include an array of redundant bar codes and a patient bed that may be spaced from the array of redundant bar codes. The patient bed may include circuitry that may comprise a bar code reader that may read at least one of the redundant bar codes in the array. The circuitry may be configured to transmit data corresponding to the at least one of the redundant bar codes and to transmit bed identifier (ID) to the network.

The array of redundant bar codes may be affixed to a vertical surface in a room of the healthcare facility. In such embodiments, the patient bed may include a frame that may have longitudinally spaced ends. The bar code reader may be mounted adjacent to one of the longitudinally spaced ends. The vertical surface may comprise a wall of the room or a panel of an architectural product that may be mounted to a wall of the room. The architectural product may include a bed locator unit, a headwall unit, or a column, for example. Alternatively or additionally, the array of redundant bar codes may be affixed to a horizontal surface in the room, such as the floor. The patient bed may include a frame and the bar code reader may be coupled to the frame so as to point downwardly toward the floor.

In some embodiments, the array of redundant bar codes may include at least one row having at least three identical bar codes. In other embodiments, the array of redundant bar codes may include at least three rows each having at least three identical bar codes. It should be appreciated that this disclosure contemplates any number of rows and columns of redundant bar codes greater or lesser in number than three.

Another system contemplated by this disclosure may include a patient bed that may have a frame, circuitry that may be carried by the frame, and a graphical user interface that may be carried by the frame and that may be coupled to the circuitry. The graphical user interface may display at least one user interface screen that may be used by a caregiver to manually enter location data that may be indicative of a location in a healthcare facility that may be occupied by the patient bed. The circuitry may transmit off of the bed the location data entered by the caregiver and a bed identification (ID).

In some embodiments, the location data may comprise a room number. The graphical user interface may include a change button that may be selected to initiate a change of the location data. A keyboard screen may appear on the graphical user interface in response to the change button being selected. The keyboard screen may permit the caregiver to type new location data that may be indicative of a new location that may be occupied by the patient bed.

In some embodiments, the system may include at least one remote computer device that may receive the location data and the bed ID for purposes of making a bed-to-room association. The patient bed may be coupled to the at least one remote computer device via a network of the healthcare facility. The location data and the bed ID may be transmitted off of the bed in the form of a wireless transmission. The circuitry also may transmit bed status data off of the bed.

In some embodiments, the location data may include unit data that may be indicative of a unit of the healthcare facility that may be occupied by the patient bed and a room number of the unit in which the patient bed may be situated. The graphical user interface may display a first screen that may be used to select the unit of the healthcare facility that may be occupied by the patient bed from a menu of units and a second screen that may be used to select the room number from a menu of room numbers.

Further according to this disclosure, a system for associating a bed to a room of a healthcare facility may include a locator unit that may be fixed in place and that may transmit a location ID. The system may include a patient bed that may have first circuitry that may have a first ID and that may receive the location ID. The patient bed may have second circuitry that may be independent of the first circuitry. The second circuitry may be configured to transmit a bed ID and bed status data.

The system may further have a first transceiver that may be spaced from the locator unit and that may be spaced from the patient bed. The first transceiver may receive the first ID and location ID transmitted by the first circuitry. A second transceiver of the system may be spaced from and independent of the first transceiver. The second transceiver may receive the bed ID and the bed status data that may be transmitted by the second circuitry.

The system may also have a first remote computer device that may receive the location ID and first ID that may be transmitted to the first remote computer device by the first transceiver. The system may further have a second remote computer device that may receive the bed ID and the bed status data which may be transmitted to the second computer device by the second transceiver. The first and second remote computer devices may cooperate to associate the location ID and the bed status data with the bed ID.

In some embodiments, the first circuitry may be included as part of a tag that may attach to an exterior surface of the patient bed. The first circuitry may transmit the first ID and the location ID using a first wireless transmission technology. The second circuitry may transmit the bed ID and the bed status data using a second wireless transmission technology. The first wireless transmission technology may differ from the second wireless transmission technology. For example, the first wireless transmission technology may comprise one of infrared technology, radio frequency technology, and ultrasonic technology and the second wireless transmission technology may comprise a different one of infrared technology, radio frequency technology, and ultrasonic technology.

Another system according to this disclosure may include a locator unit that may be fixed in place and that may transmit a location ID in a first format. The system may also include a patient bed that may have a bed ID and circuitry that may have stored therein ID translation software. The circuitry may receive the location ID in the first format and, in accordance with the ID translation software, may convert the location ID to a modified ID that may have a second format different than the first format. The circuitry may transmit the bed ID and the modified ID such that the

5

location ID received by the circuitry of the patient bed may not be transmitted by the circuitry.

The system may further include a remote computer device that may receive the bed ID and the modified ID and that may determine a location of the patient bed based on the modified ID. The modified ID may include a room number of a room in a healthcare facility in which the patient bed may be located and the translation software may include a look up table that may convert the location ID into the room number of the modified ID. The location ID may have a different number of bits of information than the modified ID.

Yet another system according to this disclosure may comprise a locator unit that may be fixed in place and that transmits a location ID. The system further may have a patient bed that may have a bed ID and circuitry that may have stored therein ID mutation software. The circuitry may receive the location ID and, in accordance with the ID mutation software, may mutate the location ID and the bed ID into a mutated ID. The mutated ID may be a single unique ID. The circuitry may transmit the mutated ID, whereby neither the location ID received by the circuitry nor the bed ID of the patient bed may be transmitted by the circuitry.

According to some embodiments, mutating the location ID and the bed ID into the mutated ID may include adding the location ID and the bed ID to create an added ID. Mutating the location ID and the bed ID into the mutated ID may further include applying a hashing function to the added ID to create a hashed ID. While any suitable hashing function is contemplated by this disclosure, in some embodiments, the hashing function may comprise a cryptographic hashing function.

The system may further comprise a remote computer device that may have decoding software that may determine the location ID and the bed ID based on the hashed ID. For example, the decoding software may include a look up table that may identify a location ID and a bed ID for each possible hashed ID. Alternatively or additionally, the decoding software may generate comparison hashed ID's by sequentially adding and hashing all known bed ID's with all known location ID's until one of the comparison hashed ID's matches the hashed ID then storing in an association database the location ID and the bed ID that caused the comparison hashed ID to match the hashed ID.

According to each of the embodiments contemplated herein, the circuitry of the patient bed may also transmit bed status data and/or a patient ID of a patient assigned to the patient bed. According to some embodiments, the remote computer device may have decoding software that determines the location ID and bed ID based on the hashed ID and that associates the location ID, bed ID and the bed status data and/or the patient ID in a database.

According to this disclosure, a method may include receiving, with circuitry on a patient bed, light from a light source that may emit visible light that may have a signature that may be unique to a location of the healthcare facility. The method may further include analyzing, using software stored in the circuitry of the patient bed, the light from the light source to determine the signature corresponding to the location, and transmitting, using the circuitry of the patient bed, data corresponding to the signature and a bed ID. In some embodiments, the method further may include receiving, with a remote computer device, the bed ID and the data corresponding to the signature and associating the location of the patient bed with the patient bed.

Another method according to this disclosure may include receiving, with circuitry on a patient bed, light from a light

6

source that may be operable to emit IR light that may have a signature that is unique to a location of the healthcare facility and that may also be operable to emit visible light. The method may further include analyzing, using software stored in the circuitry of the patient bed, the IR light from the light source to determine the signature corresponding to the location and transmitting, using the circuitry of the patient bed, data corresponding to the signature and a bed ID.

In some embodiments, the method may further include receiving, with a remote computer device, the bed ID and the data corresponding to the signature and associating the location of the patient bed with the patient bed based on the data corresponding to the signature. The IR light that may have the signature may be transmitted only when the visible light is turned off.

In some embodiments, the method further includes receiving, with the circuitry of the patient bed, visible light that may have the signature such that the visible light and the IR light may have the same signature. The signature of the visible light and/or the IR light may comprise a specified pulse frequency. As mentioned above, the specified pulse frequency may be programmable.

Yet another method according to this disclosure includes scanning, using a bar code scanner of a patient bed, at least one bar code from an array of redundant bar codes that may be mounted to a surface in a room. The bar code may be indicative of a location of the room. The method may further include transmitting off of the patient bed, using circuitry of the patient bed, data that may correspond to the at least one of the redundant bar codes and a bed ID.

In some embodiments, the method may further include receiving the data corresponding to the at least one of the redundant bar codes and receiving the bed ID at a remote computer device and associating the patient bed with the location based on the data corresponding to the at least one of the redundant bar codes and the bed ID. According to this disclosure, the surface to which the array of redundant bar codes may be mounted may comprise a surface of a room wall, a surface of architectural equipment in the room, or a floor surface.

Still another method according to this disclosure includes displaying, on a graphical user interface of a patient bed, fields that a caregiver may select to manually enter location data indicative of a location in a healthcare facility occupied by the patient bed. The method may further include receiving, on the graphical user interface, selections from the caregiver of the location data and transmitting, from the patient bed, the location data entered by the caregiver and a bed ID.

In some embodiments, the method may further comprise receiving the location data and receiving the bed ID at a remote computer device and associating the patient bed with the location based on the location data and the bed ID. The location data may comprise a room number in some embodiments and may comprise a unit number (or a unit name) and a room number in other embodiments.

Still a further method contemplated by this disclosure includes transmitting a location ID from a locator unit that may be fixed in place in a room of a healthcare facility, receiving, with first circuitry of a patient bed that may be spaced from the locator unit, the location ID. The method may further include transmitting, from the first circuitry, a first ID and the location ID and transmitting, from second circuitry of the patient bed, a bed ID and bed status data. Still further the method may include receiving, with a first transceiver that may be spaced from the locator unit and spaced from the patient bed, the first ID and location ID

transmitted by the first circuitry and receiving, with a second transceiver that may be spaced from and independent of the first transceiver, the bed ID and the bed status data transmitted by the second circuitry. The method may also include transmitting the location ID and the first ID from the first transceiver, transmitting the bed ID and the bed status data from the second transceiver, receiving, with a first remote computer device, the location ID and first ID transmitted by the first transceiver, receiving, with a second remote computer device, the bed ID and the bed status data transmitted by the second transceiver, and associating the location ID with the bed status data and the bed ID via cooperation between the first and second remote computer devices.

According to this disclosure, another method may include transmitting a location ID from a locator unit that may be fixed in place in a healthcare facility. The location ID may have a first format. The method also may include receiving the location ID with circuitry of a patient bed that may be spaced from the locator unit and that has a bed ID. The further may include converting the location ID that may have the first format to a modified ID that may have a second format using translation software that may be stored in the circuitry of the patient bed. The second format may be different than the first format. The method may include transmitting, using the circuitry, the bed ID and the modified ID, whereby the location ID received by the circuitry of the patient bed may not be transmitted by the circuitry.

In some embodiments, the method further comprises receiving, with a remote computer device, the bed ID and the modified ID and determining, with the remote computer device, a location of the patient bed based on the modified ID. The modified ID may include a room number of a room in a healthcare facility in which the patient bed may be located and the translation software on the patient bed may include a look up table that may be used to convert the location ID into the room number of the modified ID. In some embodiments, the location ID has a different number of bits of information than the modified ID.

Still another method according to this disclosure may include transmitting a location ID from a locator unit that may be fixed in place in a room of a healthcare facility, receiving the location ID in circuitry of a patient bed having a bed ID, and mutating the location ID and the bed ID into a mutated ID using ID mutation software that may be stored in the circuitry. The mutated ID may be a single unique ID. The method may further include transmitting the mutated ID from the patient bed, whereby neither the location ID received by the circuitry nor the bed ID of the patient bed may be transmitted by the patient bed.

In some embodiments, mutating the location ID and the bed ID into the mutated ID may include adding the location ID and the bed ID to create an added ID. Mutating the location ID and the bed ID into the mutated ID may further comprise applying a hashing function to the added ID to create a hashed ID. The hashing function may comprise a cryptographic hashing function, for example.

The method may further comprise determining the location ID and the bed ID based on the hashed ID at a remote computer using decoding software. The decoding software may include a look up table that identifies a location ID and a bed ID for each possible hashed ID. Alternatively or additionally, the decoding software may generate comparison hashed ID's by sequentially adding and hashing all known bed ID's with all known location ID's until one of the comparison hashed ID's matches the hashed ID then storing in an association database the location ID and the bed ID that caused the comparison hashed ID to match the hashed ID.

In some embodiments, the method may further include transmitting bed status data from the patient bed and, optionally, using a remote computer device to determine the location ID and the bed ID based on the hashed ID and to associate the location ID, bed ID and bed status data in a database. Alternatively or additionally, the method may include transmitting from the patient bed a patient ID of a patient assigned to the patient bed and, optionally, using a remote computer device to determine the location ID and bed ID based on the hashed ID and to associate the location ID, bed ID and patient ID in a database.

According to another aspect of this disclosure, a hospital bed for use with a locating and tracking system may be provided and may include a patient support structure that may be configured to support a patient. The hospital bed may further have circuitry that may be carried by the patient support structure and that may be in communication with the locating and tracking system. The hospital bed may have an indicator that may be coupled to the circuitry and that may be signaled by the circuitry to provide an indication that a successful bed-to-room association has been made.

In some embodiments, the indicator may comprise a light. The light may be turned on in response to the successful bed-to-room association being made and the light may be turned off in the absence of the successful bed-to-room association. The light may be illuminated a first color in response to the successful bed-to-room association being made and the light may be illuminated a second color in the absence of the successful bed-to-room association. The indication that a successful bed-to-room association has been made may be communicated to the circuitry from the locating and tracking system.

The hospital bed may further include an indicator module that may be attachable as a unit to the patient support structure. The indicator module may include a housing and the indicator may be carried by the housing. The circuitry may be carried by the housing. Alternatively or additionally, the indicator module may include module circuitry that may be in communication with the circuitry.

The hospital bed may have at least one other indicator. The at least one other indicator may include a communication indicator to indicate that a successful communication link has been established to a network of a healthcare facility. Alternatively or additionally, the at least one other indicator may include an alarm monitor indicator to indicate that one or more conditions of the hospital bed have been selected using a remote computer for monitoring of alarm conditions. Further alternatively or additionally, the at least one other indicator may include a signal strength indicator that may indicate a strength of a wireless communication link. For example, the signal strength indicator may comprise a multi-color light that may be illuminated different colors to indicate different levels of signal strength of the wireless communication link.

According to this disclosure, a method may include receiving at a first computer device that is remote from a bed, bed data transmitted from the bed. The method may include receiving at the first computer device, prospective bed-to-room association data transmitted from a second computer device to indicate that the bed is in a particular location, the second computer device may be included as part of a locating system. According to the method, after receiving the prospective bed-to-room association data, the first computer device may analyze the bed data to determine if it includes information indicating that a power cord of the bed is plugged into a power outlet. If the bed data includes information indicating that the power cord is plugged into a

power outlet, the method includes storing the prospective bed-to-room association data in a database associated with the first computer device as finalized bed-to-room association data.

In some embodiments, the method further includes transmitting a message from the first computer device to the bed to notify the bed that a successful bed-to-room location has been made. Alternatively or additionally, the method includes indicating on the bed that a successful bed-to-room association has been made. For example, indicating on the bed that a successful bed-to-room association has been made may comprise illuminating a light on the bed and/or displaying location information on a graphical display of the bed.

The method may further comprise detecting at the bed that the power cord has become unplugged from the power outlet and ceasing indicating on the bed that a successful bed-to-room association has been made. The method may also comprise transmitting further bed data from the bed to the first computer device. The further bed data may include information indicating that the power cord is unplugged.

In some embodiments, the method may further include disassociating the bed from the particular location at the first computer device after receiving at the first computer device the further bed data including the information that the power cord is unplugged. The method may further comprise displaying on a display screen coupled to the first computer device information to indicate that the bed-to-room association no longer exists.

According to another aspect of the present disclosure, a system may include a bed that may have bed circuitry that may be configured to control bed functions, to receive wireless signals, and to transmit signals. The system may also include a heart rate monitor that may be worn by a patient. The heart rate monitor may have monitor circuitry that may be programmed to store a medical record number (MRN) of the patient. The monitor circuitry also may be configured to transmit the MRN wirelessly to the bed circuitry. The bed circuitry may be configured to transmit bed identification (ID) data and the MRN. A first remote computer device may be configured to receive the bed ID data and the MRN of the patient and may be configured to generate patient-to-bed association data for storage in a database based on the bed ID data and the MRN.

In some embodiments, the monitor circuitry also may be configured to transmit heart rate data to the bed circuitry. The bed circuitry may be configured to transmit the heart rate data to the first remote computer device. Alternatively or additionally, the bed circuitry may be configured to transmit the heart rate data to a second remote computer device. In some embodiments, the heart rate monitor may have an arm strap that may attach to an arm of the patient. Alternatively or additionally, the heart rate monitor may have a chest strap that may attach to a chest of the patient.

According to still a further aspect of this disclosure, a system includes a bed that may have bed circuitry that may be configured to control bed functions, to receive wireless signals, and to transmit signals. The system may include a heart rate monitor that may be worn by a patient. The heart rate monitor may have monitor circuitry that may store monitor identification (ID) data. The monitor circuitry may transmit the monitor ID data wirelessly to the bed circuitry. The bed circuitry may, in turn, transmit bed identification (ID) data and the monitor ID data. The system may further have a first remote computer device that may receive the bed ID data and the monitor ID data, that may correlate the monitor ID data with a medical record number (MRN) of the

patient and that may generate patient-to-bed association data for storage in a database based on the bed ID data and the MRN.

In some embodiments, the monitor circuitry also may be configured to transmit heart rate data to the bed circuitry. In such embodiments, the bed circuitry may be configured to transmit the heart rate data to the first remote computer device. Alternatively or additionally, the bed circuitry may be configured to transmit the heart rate data to a second remote computer device. In some embodiments, the heart rate monitor may have an arm strap that attaches to an arm of the patient. Alternatively or additionally, the heart rate monitor may have a chest strap that attaches to a chest of the patient.

According to yet another aspect of this disclosure, a system may comprise a bed may have a first radio frequency (RF) communication module that may have first identification (ID) data. The first RF communication module may transmit bed data and the first ID data wirelessly from the bed. The bed may have a power cord that carries a transponder. The system may further include a second RF communication module that may be spaced from the bed and situated adjacent to a wall of a room in which the bed is located. The second RF communication module may have second ID data. The second RF communication module may receive the bed data and first ID data transmitted wirelessly from the first RF communication module of the bed.

The system may also have a transponder reader that may be situated adjacent to the wall of the room and that may be configured to read wireless information from the transponder including the first ID data. The system may include a communication circuit that is situated adjacent to the wall of the room. The communication circuit may be coupled to the transponder reader and coupled to the second RF communication module. The communication circuit may be configured to receive the first ID data from the transponder reader and to receive the second ID data from the second RF communication module. The communication circuit may pair the first and second RF communication modules so that the second RF communication module only accepts communication packets from the first RF communication module. Alternatively or additionally, the communication circuit may pair the first and second RF communication modules so that the communication board only accepts communication packets from the second RF communication module if the packets contain the first ID data.

In some embodiments, the bed may further include a Wi-Fi communication module. In such embodiments, the first RF communication module and the Wi-Fi communication module may be controlled so as to send wireless transmissions in different, non-overlapping time slots. In some embodiments, the communication circuit may be configured to send the bed data received via the first and second RF communication modules to a remote computer device.

The system may further have a data cable that may extend from the bed and which may be coupleable to the communication circuit. Thus, the communication circuit may receive the bed data transmitted by the bed over the data cable when the communication circuit is coupled to the data cable. The communication circuit may cease to accept bed data from the second RF communication module and may accept only the bed data transmitted over the data cable. In some embodiments, the bed may include a siderail and the first RF communication module may be coupled to the siderail.

The transponder may comprise an RFID tag, if desired. For example, the RFID tag may be molded into a plug body of the power cord or may be situated on a label attached to the power cord. The transponder reader may comprise a loop antenna. The loop antenna may be located adjacent a power outlet to which the power cord couples.

Further according to this disclosure, a system may include a bed that may have a first radio frequency (RF) communication module that may have first identification (ID) data and a second RF communication module that may have second ID data. The first and second RF communication modules may transmit bed data and the respective first and second ID data wirelessly from the bed. The bed may have a power cord that may carry a transponder. A third RF communication module may be spaced from the bed and situated adjacent to a wall of a room in which the bed is located. The third RF communication module may have third ID data. The third RF communication module may receive wireless transmissions from the first and second RF communication modules of the bed. The wireless transmissions may include the bed data and the respective first and second ID data transmitted wirelessly.

The system may further have a transponder reader that may be situated adjacent to the wall of the room and that may be configured to read wireless information from the transponder including the first ID data and the second ID data. A communication circuit of the system may be situated adjacent to the wall of the room. The communication circuit may be coupled to the transponder reader and may be coupled to the third RF communication module. The communication circuit may be configured to receive the first and second ID data from the transponder reader and to receive the third ID data from the second RF communication module. The communication circuit may pair the first and second RF communication modules with the third RF communication module so that the third RF communication module only accepts communication packets from the first communication module or the second communication module.

In some embodiments, the third RF communication module may be configured to assess signal strength of the wireless transmissions from the first and second RF communication modules and to communicate only with the first or second RF communication module that may have greater signal strength. Thus, the third RF communication module may operate as a master and the first and second RF communication modules may each operate as a slave. If the third RF communication module is unable to communicate with the first and second RF communication modules, then an alarm may be triggered by the third RF communication module.

In some embodiments, the bed may further include a Wi-Fi communication module. The first and second RF communication modules and the Wi-Fi communication module may be controlled so as to send wireless transmissions in different, non-overlapping time slots. The communication circuit may be configured to send the bed data received via the third RF communication module to a remote computer device.

The system may further include a data cable which may extend from the bed and which may be coupleable to the communication circuit. The communication circuit may receive the bed data transmitted by the bed over the data cable when the communication circuit is coupled to the data cable. The communication circuit may be configured to cease accepting bed data from the third RF communication module and to accept the bed data transmitted over the data

cable. The bed may include a first siderail and a second siderail. The first RF communication module may be coupled to the first siderail and the second RF communication module may be coupled to the second siderail.

In the system having the first, second and third communication modules, the transponder may comprise an RFID tag such as one molded into a plug body of the power cord or on a label attached to the power cord. In such a system, the transponder reader may comprise a loop antenna such as one that may be located adjacent a power outlet to which the power cord couples.

Still further according to this disclosure, a bed-to-room association system may comprise a bed that may have a power cord that may carry a first RFID component and a receptacle module that may carry a second RFID component. The receptacle module may have a receptacle into which the power cord may plug to receive power and to bring the first and second RFID components into communicative proximity. The receptacle module may have an indicator that may be activated in response to successful communication being established between the first and second RFID components.

In some embodiments, the indicator may comprise a light. The light may comprise a light ring, for example. The light ring may surround the receptacle. The first RFID component may comprise one of an RFID tag and an RFID reader and the second RFID component may comprise another of the RFID tag and RFID reader.

Also according to this disclosure, an apparatus for communicating with a nurse call system of a healthcare facility may be provided. The apparatus may include a bed that may have a first transceiver for wireless communication of bed identification (ID) data and bed status data. The apparatus may also include a handheld pillow speaker unit that may have a second transceiver in wireless communication with the first transceiver. The pillow speaker unit may be in hardwired communication with the nurse call system. Thus, the pillow speaker unit may serve as a communication intermediary between the bed and the nurse call system.

In some embodiments, the apparatus may further include an interface unit that may be fixed with respect to a wall in a patient room. The pillow speaker unit may have a cable with a plug that may plug into the interface unit. The interface unit may be communicatively coupled to the nurse call system.

The pillow speaker unit may include a first set of user inputs that may be used to control at least one of the following: a television, a room light, and at least one window shade. The bed may include a second set of user inputs that may be used to control at least one of the following: the television, the room light, and the at least one window shade.

In some embodiments, use of the second set of user inputs may be communicated from the first transceiver of the bed to the second transceiver of the pillow speaker unit. Thus, the pillow speaker unit may include user inputs that are used to control bed functions.

It is contemplated by this disclosure that the pillow speaker unit may include a set of manual buttons and a touchscreen graphical display that displays electronic buttons. The manual buttons may include at least one of the following: a nurse call button, a reading light button, and a room light button. The manual buttons may further include at least one of the following: a television control button, a radio control button, and a telephone dial pad button. The electronic buttons may include buttons that may be used to send distinct preprogrammed messages to at least one care-

13

giver. At least one of the manual buttons and at least one of the electronic buttons may control a same function.

According to a further aspect of the present disclosure, a pillow speaker unit that may communicate with a nurse call system in a healthcare facility is provided. The pillow speaker unit may include a handheld housing, a set of manual buttons that may be accessible on the housing, and a touchscreen graphical display that may display electronic buttons. At least one of the manual buttons and at least one of the electronic buttons may be usable to send a respective signal to the nurse call system. The pillow speaker unit may include the features discussed previously.

Additional features, which alone or in combination with any other feature(s), such as those listed above and/or those listed in the claims, may comprise patentable subject matter and will become apparent to those skilled in the art upon consideration of the following detailed description of various embodiments exemplifying the best mode of carrying out the embodiments as presently perceived.

BRIEF DESCRIPTION OF THE DRAWINGS

The detailed description particularly refers to the accompanying figures in which:

FIG. 1 is perspective view of a patient bed having a sensor that receives light emitted from an overhead display screen (in solid) or from a wall-mounted display screen (in phantom), the light having a signature (indicated diagrammatically via a square wave) that is unique for the location occupied by the bed, the bed having circuitry (shown diagrammatically) that analyzes the signature and transmits data corresponding to the signature and transmits a bed identifier (ID) to one or more remote computer devices (shown diagrammatically) via a network (shown diagrammatically)

FIG. 2 is a diagrammatic perspective view showing a number of light bulbs that each emit light having a unique signature, each bulb being associated with a different room, and showing a sensor receiving the light and signature from a first bulb, the bed having circuitry that analyzes the signature and transmits data corresponding to the signature and transmits a bed ID to one or more remote computer devices via the network;

FIG. 3 is a perspective view of an alternative embodiment of a patient bed having a bar code scanner (shown diagrammatically) that scans at least one bar code of an array of redundant bar codes that is affixed to a floor surface, the bed having circuitry (shown diagrammatically) that is coupled to the bar code scanner and that transmits data corresponding to the at least one bar code and bed ID to the network;

FIG. 4 is a partial perspective view of a bed, similar to that of FIG. 3, having a bar code scanner (shown diagrammatically) that scans at least one bar code of an array of redundant bar codes that is affixed to a vertical surface of a bed locator unit, the bed having circuitry (shown diagrammatically) that is coupled to the bar code scanner and that transmits data corresponding to the at least one bar code and bed ID to the network;

FIG. 5 is a diagrammatic view showing a graphical user interface (GUI) of a bed having a touch screen display that displays a room number and a change button, the bed being coupled to one or more remote computer devices via a network and the bed transmitting the room number and a bed ID to the one or more remote computer devices via the network;

FIG. 6 is a diagrammatic view, similar to FIG. 5, showing a keypad that appears on the GUI after selection of the

14

change button, the keypad being usable by a caregiver to enter a new room number corresponding to a new location of the bed;

FIG. 7 is a diagrammatic view, similar to FIG. 5, showing the new room number being displayed on the GUI, the new room number and bed ID being transmitted by the bed to the one or more remote computer devices via the network.

FIG. 8 is a diagrammatic view of an alternative embodiment showing the GUI displaying a menu of unit ID's that appear on a drop down menu in response to selection of the change button;

FIG. 9 is a diagrammatic view, similar to FIG. 8, showing the GUI displaying a menu of room ID's that appear on a drop down menu in response to selection of the unit ID on the GUI screen of FIG. 8;

FIG. 10 is a diagrammatic view showing a Confirm Association screen that appears on the GUI after the unit ID and room ID have been selected, a yes button that is selected by the caregiver to confirm the association of the bed to the selected unit and the selected room, the bed transmitting the selected unit ID and the selected room ID, along with a bed ID, to the one or more remote computer devices via the network;

FIG. 11 is a flow chart of an algorithm of the bed that is embodied in software and that is executed to permit selection of the unit ID and the room ID by the caregiver;

FIG. 12 is a diagrammatic view showing a patient bed having a tag that receives a locator ID from a fixed location unit and that transmits a tag ID and the locator ID to a first transceiver that, in turn, transmits via a network the tag ID and the locator ID to a first remote computer device, the patient bed having circuitry that transmits a bed ID and bed status data to a second transceiver that, in turn, transmits via the network the bed ID and the bed status data to a second remote computer device, and the first and second computer devices being communicatively coupled so as to cooperate to associate the location ID and the bed status data with the bed ID;

FIG. 13 is a diagrammatic view showing a locator unit transmitting a location ID_A, a bed receiving location ID_A and having ID translation software stored in bed circuitry that converts location ID_A to location ID_B, the bed transmitting a bed ID and location ID_B to at least one remote computer device via a network, whereby the location ID_A received by the circuitry of the patient bed is not transmitted by the circuitry;

FIG. 14 is a diagrammatic view showing a locator unit transmitting a location ID, a bed having circuitry receiving the location ID and having ID mutation software that is stored in the circuitry and that mutates the location ID and a bed ID into a mutated ID that is a single unique ID that is transmitted by the circuitry of the bed to at least one remote computer device via a network, the remote computer device having ID decoding software that determines the location ID and bed ID that corresponds to the mutated ID;

FIG. 15 is a perspective view showing an indicator module exploded away from a hospital bed, the indicator module having three LED's, one of which is illuminated to indicate that a successful bed-to-room association has been made;

FIG. 16 is a block diagram of a wireless bed-to-room association system similar to that of FIG. 12 showing that location information is transmitted from a remote server to the circuitry of the hospital bed;

FIG. 17 is a flow chart showing an algorithm of a portion of the software executed by the remote server of the system of FIG. 16 in which the remote server first confirms that the

15

hospital bed is plugged into an AC outlet prior to sending the location information to the circuitry of the hospital bed;

FIG. 18 is a flow chart showing a disassociation algorithm implemented by the hospital bed and remote server of FIG. 16 in response to the hospital bed being disconnected from an AC power outlet;

FIG. 19 is a diagrammatic view showing a patient-to-bed association system in which a wireless heart rate monitor sends data, including the patient's medical record number (MRN), to circuitry of a hospital bed which, in turn, transmits the patient's MRN and a bed ID for used by a remote computer device to associate the patient to the bed;

FIG. 20 is a block diagram of another bed data system in which a bed equipped with one or two bed Bluetooth (BT) modules communicates with a wall BT module for transmission of bed data after a BT pairing operation is conducted based on transmission of bed BT module ID data via a transponder carried by a plug of a power cord of the hospital bed;

FIG. 21 is a block diagram showing a prior art bed that lacks any BT modules still being usable with the system of FIG. 20;

FIG. 22 is a block diagram similar to FIG. 21 but having a network interface unit (NIU) with two 37-pin cable connection ports so that a cable from a wall communication board remains plugged into one of the ports of the NIU even when a prior art bed has its 37-pin cable plugged into the other port of the NIU;

FIG. 23 is a perspective view showing a first AC power cord having an RFID tag molded into a plug body and showing a second AC power cord having an RFID tag included in a label that attaches to a cord portion adjacent a plug body;

FIG. 24 is a perspective view showing an AC cord having a plug that carries a first RFID component and a receptacle module having a second RFID component, a light-up ring is provided around a receptacle of the receptacle module and is illuminated when a successful bed-to-room association has been made;

FIG. 25 is a diagrammatic cross-sectional view of the AC cord of FIGS. 23 and 24;

FIG. 26 is a diagrammatic view of a further bed-to-room association system in which wireless communication is established between circuitry of a bed and a handheld pillow speaker which acts as a communication intermediary between the bed and a nurse call system as well as one or more other remote computer devices;

FIG. 27 is a front elevation view of a first embodiment of a handheld pillow speaker unit showing the pillow speaker unit having a graphical user interface (GUI) with touchscreen buttons and a number of manual buttons beneath the GUI; and

FIG. 28 is a front elevation view of a second embodiment of a handheld pillow speaker unit showing the pillow speaker unit having a GUI with touchscreen buttons, a manual nurse call button beneath the GUI, a first on/off button for control of a first light, and a second on/off button for control of a second light.

DETAILED DESCRIPTION

Throughout FIGS. 1-28, a bed 20 has circuitry 22 that transmits data of various types in various embodiments as discussed below via a network 24 to one or more remote computer devices 26. FIGS. 1-4, 13 and 14 each show a diagrammatic transmitter 28 that is coupled to, or included as part of, circuitry 22. It should be understood that each bed

16

20 has a transmitter of some type, such as illustrative transmitter 28 which, in some embodiments, is included as part of a transceiver. It is contemplated by this disclosure that transmitter 28 transmits data wirelessly, but that is not to say that transmitter 28 is excluded from sending data over a wired connection to network 24 in contemplated embodiments, if desired. In FIGS. 15 and 16, modules 150, 150', respectively, are included on bed 20 and have wireless communication capability. In FIG. 20, a first module 232 and an optional, second module 234 are included on bed 20 and have wireless communication capability. In FIG. 26, bed 20 has a module 150" with wireless communication capability.

While circuitry 22 is shown in the various figures as a single diagrammatic block, it should be understood that the single block is intended to represent all of the circuitry found on a patient bed and such circuitry may be embodied in separate, but interconnected, modules and/or circuit boards. In other words, circuitry 22 of patient bed 20 comprises a large complex circuit. See, for example, "Service Manual, Progressa™ Bed From Hill-Rom," © 2013, Hill-Rom Services, Inc.; "Service Manual, TotalCare® Bed System From Hill-Rom," © 2008, Hill-Rom Services, Inc.; and "Service Manual, VersaCare® Bed From Hill-Rom," 2008, Hill-Rom Services, Inc.; each of which is hereby incorporated by reference herein. See also U.S. Pat. Nos. 5,771,511 and 7,506,390, each of which is hereby incorporated by reference herein.

Furthermore, network 24 (aka Ethernet 24 in FIGS. 13 and 14) is represented diagrammatically by a cloud image in the various figures. This image is intended to represent all of the hardware components and software that make up various types of networks in a healthcare facility. The architecture and functionality of such networks can vary widely. Suffice it to say that, in some embodiments, the networks 24 contemplated herein have wireless access points for wireless connectivity to the network by various devices, including bed 20. Alternatively or additionally, networks 24 contemplated herein have ports, such as ports that receive RJ-45 connectors, for wired connection of various devices, including bed 20, to the respective network 45. Thus, network 24 includes, for example, computer devices such as nurse call computers, electronic medical records (EMR) computers, admission/discharge/transfer (ADT) computers, and the like. Examples of the type of communication equipment included in various embodiments of a nurse call system (as well as network 24, in general) can be found in U.S. Pat. Nos. 8,598,995; 8,384,526; 8,169,304; 8,046,625; 7,746,218; 7,538,659; 7,319,386; 7,242,308; 6,897,780; 6,362,725; 6,147,592; 5,838,223; 5,699,038 and 5,561,412, all of which are hereby incorporated by reference herein in their entirety to the extent that they are not inconsistent with the present disclosure which shall control as to any inconsistencies.

The various embodiments disclosed herein relate to systems and methods for making bed-to-room associations in a healthcare facility. This is accomplished by associating a bed identifier (ID) and a location identifier (ID) in a database of a computer device 26, such as a server or other computer. The term "room" in the phrase "bed-to-room" is intended to include not just patient rooms, but also hallways, service areas, supply rooms, elevators, cleaning rooms, and any other location in a healthcare facility which may be occupied by a bed. In each of the embodiments disclosed herein, other types of data may also be associated with the bed and/or room in the database, such as a patient ID, bed status data, data from other types of medical equipment (e.g., IV pumps,

therapy equipment, vital signs equipment, and so forth), and data from other medical systems (e.g., electronic medical records (EMR) system, admission/discharge/transfer (ADT) system, pharmacy system, laboratory system, and so forth). Thus, patient-to-room; patient-to-bed; and patient-to-bed-to-room systems and methods are contemplated herein. It should also be appreciated that the order of association makes no difference and that “bed-to-room” and “room-to-bed” associations mean the same thing and that “patient-to-bed-to-room” and “room-to-patient-to-bed” associations mean the same thing, just to give a couple examples.

Referring now to FIG. 1, bed 20 has a sensor 30 that receives light emitted from an overhead display screen 32. In an alternative embodiment, screen 32 is omitted and the light received by sensor 30 is emitted from a wall-mounted display 34 screen (in phantom). Screen 32, in some embodiment, is operated to display one or more nature scenes that are conducive to a patient's recovery and/or one or more night sky scenes that are conducive to helping the patient fall asleep. Screen 34, in some embodiments, is included as part of a room station of a nurse call system or as part of some other computer device in the room.

The light emitted from screens 32, 34 is visible light that has a signature 36 (indicated diagrammatically via a square wave). The signature 36 is unique for the location occupied by the bed 20. That is, the signature of the light emitted from screens 32, 34 is different for different rooms. Circuitry 30 is coupled to sensor 30 and analyzes the emitted light to determine its signature 36. In some embodiments, sensor 30 comprises a camera and in other embodiments, sensor 30 comprises a red-green-blue (RGB) image sensor chip. The signature 36 is emitted at a specified wavelength and/or at a specified pulsed frequency. The pulsed frequency is sufficiently large and/or the wavelength is sufficiently short in duration so as to be imperceptible to human vision. The specified wavelength and/or the specified pulse frequency is unique to each room. Thus, by analyzing the emitted light to determine the signature 36, data corresponding to the signature 36 is usable to determine the location of bed 20 in the associated healthcare facility.

Circuitry 22 commands transmitter 28 to transmit data corresponding to the signature and also commands transmitter 28 to transmit a bed identifier (ID) to at least one remote computer device 26 via a network 24. Typically, the data corresponding to the signature and the bed ID are included in the same message packet. The remote computer device 26 then makes the bed-to-room association based on the data corresponding to the signature and the bed ID. Thus, the remote computer device 26 includes a table or other similar type of relational database that correlates the data corresponding to the signature with a particular location, such as a patient room number, in the healthcare facility.

Referring now to FIG. 2, light bulbs 38a-e are shown diagrammatically and each light bulb 38a-e emits light having a unique signature. It should be understood that each bulb 38a-e is located in a different room of the healthcare facility. In the illustrative example of FIG. 2, bulb 38a is in communication with bed 20. Thus, sensor 30 receives the light and signature from a first bulb 32a as indicated diagrammatically in FIG. 2 with dashed arrow 39. Just like the embodiment of FIG. 1, circuitry 22 of bed 20 analyzes the emitted light to determine the signature and transmits data corresponding to the signature and transmits bed ID to at least one remote computer device 26 via the network 24 and computer device 26 makes the bed-to-room association based on the received signature data and bed ID.

In some embodiments, bulbs 38a-e are high-power white LED lightbulbs that are programmable to emit a specified wavelength at a specified pulsed frequency. For example, bulbs 38 are programmable to emit different percentages of blue, red and green light (e.g., 11% blue, 30% red, and 59% green) which still appear generally as white light. In some embodiments, the bulb 38a-e in each room emit the same percentage of blue, red and green light, but at a different pulsed frequency for each room. In some embodiments, sensor 30 is embodied as a simple photovoltaic sensor and the unique light signatures are created by varying a power duty cycle of the associated light source without regard to wavelength. For example, the light source is turned on and off (e.g., flickered) at a specified frequency which is imperceptible to human vision but which is unique to each room.

Suitable programmable bulbs 38a-e are available from ByteLight of Boston, Mass. See also, U.S. Pat. Nos. 8,520,065; 8,457,502; 8,436,896; 8,432,438; 8,416,290; 8,334,901; 8,334,898; and 8,248,467; each of which is hereby incorporated by reference herein.

In some embodiments, in order to enable locating to take place in rooms that have the light source turned off, a source of infrared (IR) light is emitted with a signature and sensed by sensor 30. The processing thereafter is the same as described above with regard to signatures included in the light emitted from screens 32, 34 and bulbs 38a-e. The IR light pulses, in some embodiments, are at a lower frequency which is possible because IR light is not visible to humans anyway. Thus, a visible light signature and an IR light signature may each indicate the same room, although their pulsed frequencies are different. In other embodiments, the IR light pulses are at the same pulsed frequency as the visible light pulses. In any event, it should be understood that the IR light signatures are different from room to room.

A lower amount of power is used to drive the IR light sources when the light sources of visible and IR light are in night mode. While it is possible for the IR light source to be separate from the light sources described above, it is contemplated by this disclosure that the IR light source is included in the same light source that emits visible light when in the on state. In such embodiments, when the visible light source is turned on, some of the applied power is stored in a battery or capacitor or other energy storage device and is used to drive the IR light source after the visible light source is turned off. In some embodiment, therefore, the IR light source only operates when the visible light is turned off. In other embodiments, the IR light source operates all the time.

In some embodiments, bed 20 includes two sensors 30, one for the visible light and one for the IR light. However, combined RGB and IR image or light sensors are known in the art. See, for example, U.S. Patent Application Publication No. 2010/00289885 which is hereby incorporated by reference herein. Such a device or similar such devices may be used as the sensor 30 of bed 20 if desired.

Referring now to FIG. 3, bed 20 has a bar code scanner 40 that scans at least one bar code 42 of an array 44 of redundant bar codes 42 that are affixed to a floor surface 46 of other horizontal surface. In some embodiments, array 44 of bar codes 42 is included on a floor mat that lies on the floor 46 and, in other embodiments, array 44 of bar codes 42 is included on a label that sticks to the floor 46. In still other embodiments, bar codes 42 are included on one or more floor tiles that form part of the floor surface. Circuitry 22 commands transmitter 28 to transmit data corresponding to the at least one bar code 42 and a bed ID to one or more remote computer devices 26 via the network 24. The bed-

19

to-room association is then made by the remote computer device 26 based on the data corresponding to the at least one bar code 42 and the bed ID. Having redundant bar codes 42 is an improvement over prior art system that may have only one bar code to be read by a bar code scanner. This is because the bed 20 does not need to be as precisely placed within the hospital room. Scanner 40 just needs to read one of the bar codes 42 of the array 44. In the illustrative example of FIG. 3, scanner 40 is mounted to an upper frame of the overall bedframe of bed 20 and scans downwardly through a large opening defined by frame members of a base frame of the bedframe of bed 20.

Referring now to FIG. 4, bed 20 has a bar code scanner 40' mounted to its upper frame and arranged to scan at least one bar code 42 of an array 44 of redundant bar codes 42 that is affixed to a vertical surface 48 of a bed locator unit 50 that is mounted to a room wall 52. In other embodiments, array 44 is affixed to room wall 52 or to a panel 54 of a piece of architectural equipment, such as, for example, the illustrative column 56, a headwall unit or an arm. Circuitry 22 commands transmitter 28 to transmit data corresponding to the at least one bar code 42 read by scanner 40' and a bed ID to one or more remote computer devices 26 via the network 24. The bed-to-room association is then made by the remote computer device 26 based on the data corresponding to the at least one bar code 42 and the bed ID. Having redundant bar codes 42 on a vertical surface, such as illustrative surface 48, is an improvement over prior art system that may have only one bar code to be read by a bar code scanner. By having redundant bar codes 42, the bed 20 does not need to be as precisely placed within the hospital room. Scanner 40' just needs to read one of the bar codes 42 of the array 44. In the illustrative example of FIG. 4, scanner 40' is mounted to an upper frame of the overall bedframe of bed 20 and scans generally horizontally outwardly from a head end of the bed 20.

Although only one row is included in the array 44 of FIG. 4, it will be appreciated that multiple rows are within the scope of this disclosure. Having multiple rows permits upper frame of bed 20 to be adjusted many different heights and yet scanner 40' can still read one of the bar codes 42 of the multi-row array. Furthermore, while array 44 of FIG. 4 has five bar codes 42 and while each row of array 44 of FIG. 3 has three bar codes, embodiments having more or less bar codes 42 than three or five in any given row are within the scope of this disclosure. Moreover, arrays 42 having any number of rows greater than one are within the scope of this disclosure, the upper limit being bounded primarily by the size of the bar codes 42 and the size of the surface against which the array 44 is placed.

Referring now to FIGS. 5-7, in an alternative embodiment according to this disclosure, bed 20 has a graphical user interface (GUI) 60 with a touch screen display 62 that displays a current room number, here "237," and a change button 64 on a home screen as shown in FIG. 5. As with the other embodiments disclosed herein, bed 20 of FIGS. 5-7 is coupled to one or more remote computer devices 26 via network 24 and the remote computer device(s) 26 make bed-to-room associations based on received location ID and bed ID.

In response to a caregiver selecting change button 64 on GUI 60, a keypad 66 appears on the GUI 60. The text "Enter Room Number" appears above keypad 66 in the illustrative example to suggest to the caregiver that a new room number be entered into the memory of circuitry 22 to replace the old room number. In the illustrative example, keypad 66 includes buttons having numbers 0-9 arranged in similar

20

manner as a standard telephone, a back button 68, an enter button 70, and cancel button 72. In other embodiments an alphanumeric keyboard is provided to permit the user to indicate whether the bed is at an "A" location or a "B" location in a semi-private room for example.

Keypad 66 is used by a caregiver to enter the room number in which bed 20 is located into the memory of circuitry 22 of bed 20. Circuitry 22 of bed 20 then transmits the room number in any suitable format along with the bed ID to one or more remote computer devices 26 via network 24. Thus, the room number manually entered by the user or caregiver serves as the location ID for the respective bed 20. Bed 20 does not rely on any external device or artifact (e.g., light source, locator unit, bar code label, etc.) for obtaining the location ID to be transmitted from the bed 20. Accordingly, the embodiment of FIGS. 5-7, as well as the alternative embodiment of FIGS. 8-11 discussed below, are the lowest cost embodiments contemplated by this disclosure.

In the example of FIG. 6, the caregiver has entered a new room number, here "103," using keypad 66. If the caregiver wishes to revise the entered number, the back button 68 is selected and a revised digit can be entered by the caregiver using one of the numeric keys of keypad 66. If the caregiver is satisfied that the correct room number is entered, the caregiver selects the enter key 70. If the caregiver wishes to abort the room number change altogether, the caregiver selects the cancel key 72. After the enter key 70 is selected, GUI 60 returns to the home screen, as shown in FIG. 7, but having the new room number displayed on screen 62. Thereafter, circuitry 22 of bed 20 transmits the new (now the current) room number as the location ID rather than the old room number.

Referring now to FIG. 8, in some embodiments, after selection of the change button 64 of FIG. 5, an alternative screen appears on GUI 60 and on this alternative screen is displayed a menu of unit ID's, such as a drop down menu. The user then selects the desired unit by touching the display screen 62 over the text corresponding to the desired unit. In the illustrative example, the text "Unit 1," "Unit 2," and "Unit 3" appears in menu 74, but other unit names such as ICU, NICU, Med/Surg, Neurology, Pediatrics, and so forth, just to name a few, are within the scope of this disclosure. The text appearing in menu 74 is dictated by the programming of the software stored in circuitry 22 of bed 20. A cancel button 75 appears beneath menu 74 in the FIG. 8 example and is selected by a caregiver to abort changing the location ID of bed 20.

In response to selection of the desired unit from unit menu 74 of FIG. 8, a room menu 76 appears on screen 62 of GUI 60 as shown in FIG. 9. Room menu 76 lists the rooms that are within the unit selected from menu 74. In the illustrative example, the text "Room 101A," "Room 101B," and "Room 102" appears in menu 76, but other room identifiers are within the scope of this disclosure. The text appearing in menu 76 is dictated by the programming of the software stored in circuitry 22 of bed 20. Cancel button 75 also appears beneath menu 76 in the FIG. 9 example and is selected by a caregiver to abort changing the location ID of bed 20. By providing one or both of menus 74, 76, rather than keypad 66, caregivers are only able to select location designators that are in the pre-approved format. In other words, it might be possible for caregivers to use keypad 66 to enter an erroneous room designation or to enter a room number that doesn't exist. By having menus 74, 76 with options from which caregivers select, the possibility for unit/room ID errors is minimized.

21

In response to selection of the desired room from room menu 76 of FIG. 9, a Confirm Association screen 78 appears on the GUI 60 as shown in FIG. 10. In the illustrative example of FIG. 10, there is text indicating that “Unit 1” was selected by the caregiver from menu 74 and “Room 101A” was selected by the caregiver from menu 76. Screen 78 includes a yes button 80 that is selected by the caregiver to confirm the association of the bed 20 to the selected unit and the selected room. The unit and room information, therefore, becomes the location ID for bed 20 in response to button 80 being selected. Bed 20, thereafter, transmits the selected unit ID and the selected room ID (now, the location ID), along with a bed ID, to one or more remote computer devices 26 via the network 24 and the one or more remote computer device(s) makes the bed-to-room association based on those ID’s. Screen 78 has a Try again button 82 that the caregiver selects to return to the screen of FIG. 8 having the unit menu 74 to start the process anew. Screen 78 also has the back button 75 that is selected by the caregiver to abort the room change operation and return to the home screen of FIG. 5, for example.

Referring now to FIG. 11, a flow chart 90 is provided and is illustrative of software that is executed, in some embodiments, by bed 20 and by a remote server 26 to permit selection of the unit ID and the room ID by the caregiver in response to AC Power being applied or after a new patient arrives at the bed. In the embodiment contemplated by the flow chart of FIG. 11, bed 20 is capable of two way communication with the remote computer device or server 26. Accordingly, as indicated at block 84, after AC power is applied to the bed 20 (e.g., a power cord of the bed gets plugged into an AC outlet after having been unplugged) or after a new patient arrives at the bed 20, bed 20 queries the server for an association database as indicated at block 86. Thus, prior to use of bed 20, a server configuration is performed at the server 26 as indicated at block 88 of flow chart 90. During the server configuration, association data indicative of which rooms are included as part of each unit are entered into a database of server as indicated at block 92 until complete as indicated at block 94, at which point an association database exists for use by bed 20 as indicated at block 96. In some embodiments, prior bed-to-room associations are also populated in the association database of block 96.

After bed 20 queries server 26 for the existence of the association database, bed 20 proceeds to block 98 and determines whether the bed 20 is associated with a location, which in this example means the bed 20 is associated with a unit and a room. If there is no bed-to-location association in the database, then bed 20 proceeds to block 100 and the screen of FIG. 8 is presented to the caregiver on GUI 60 for selection of the appropriate unit occupied by the bed 20. After unit selection, bed 20 proceeds to block 102 and the screen of FIG. 9 is presented to the caregiver on GUI 60 for selection of the appropriate room occupied by the bed 20. After room selection, bed 20 proceeds to block 104 and the Confirm Association screen of FIG. 10 is presented to the caregiver on GUI 60. As indicated at block 106, if the caregiver selects the yes button 80, bed 20 proceeds to update the association database as indicated at block 108 such as by, for example, transmitting the bed ID and the manually entered location ID to the server 26 via network 24. At that point, the bed is associated with the location (room and unit in this example) as indicated at block 110.

If at block 106, the caregiver selects the Try again button 82, bed 20 proceeds back to block 100 as indicated in FIG. 11 and the software algorithm proceeds from there as

22

already discussed above. If at block 106, the caregiver selects the cancel button 75, the bed 20 is not associated with any location and the association database is updated to indicate that there is no location associated with the bed. In some embodiments, further notifications are displayed on screen 62 of GUI to advise the caregiver that the bed is not associated and that the caregiver should try again by selection of button 82.

If at block 98 bed determines that it is associated with a location in the association database, bed 20 proceed to block 112 and determines how long the bed 20 experienced the AC power loss, such as being unplugged. As indicated at block 114, if the power loss was less than two minutes, then bed proceeds to block 110 and the prior bed-to-location association is maintained. If the power loss was more than two minutes, as determined at block 114, then Confirm Association screen 78 of FIG. 10 is presented to the caregiver on GUI 60 so that the caregiver can confirm the bed to location association or change it. As indicated in a notes block 116 of FIG. 11, in some embodiments, a universal serial bus (USB) stick is used in lieu of or in addition to the server 26 to store the association database. Thus, in some embodiments, the association database is loaded periodically into the memory of circuitry 22 of bed 20 using a USB stick or other similar type of portable memory device.

Referring now to FIG. 12, bed 20 has separate circuitry that communicates with first and second remote computer devices 26a, 26b via separate and generally parallel communication channels. According to this disclosure, first circuitry of bed 20 is included on a locating tag 118 that is affixed to bed 20 to be transported therewith. A locator or location unit 120 is mounted at a fixed location unit in the room, such as on a room wall, and transmits a locator ID to the tag 118. The tag 118 transmits a tag ID and the locator ID to a first transceiver 122 that, in turn, transmits via network 24 the tag ID and the locator ID to the first remote computer device 26a. Circuitry 22 of bed 20 serves as the second circuitry in this embodiment and transmits a bed ID and bed status data to a second transceiver 124 that, in turn, transmits via the network 24 the bed ID and the bed status data to the second remote computer device 26b. The first and second computer devices 26a, 26b are communicatively coupled, as indicated by the double headed arrow 126, so as to cooperate to associate the location ID and the bed status data with the bed ID. The association can occur in computer device 26a, computer device 26b, or both.

It is contemplated by this disclosure that the first circuitry of tag 118 transmits the first ID and the location ID using a first wireless transmission technology and that the second circuitry, here circuitry 22 of bed 20, transmits the bed ID and the bed status data using a second wireless transmission technology that is different than the first wireless transmission technology. For example, the first wireless transmission technology may comprise one of infrared (IR) technology, radio frequency (RF) technology, and ultrasonic (US) technology and the second wireless transmission technology comprises a different one of IR technology, RF technology, and ultrasonic technology.

Referring now to FIG. 13, a further embodiment according to this disclosure includes a locator unit 130 that is mounted to a fixed location in a healthcare facility. Unit 130 has circuitry 132 with a transmitter 134 that is commanded by circuitry 132 to transmit a first location ID, which in the illustrative example is designated as location ID_A. Circuitry 22 of bed 20 receives location ID_A and has ID translation software 136 that is stored in circuitry 22 and that converts location ID_A to a second location ID (sometimes referred to

23

herein as a modified ID), which in the illustrative example is designated as location ID_B. For example, in some embodiments, the modified ID is or includes a room number of a room in a healthcare facility in which the patient bed is located and the translation software 136 includes a look up table that correlates the location ID with the room number of the modified ID. Thereafter, circuitry 22 of bed 20 commands transmitter 28 to transmit a bed ID and location ID_B (i.e., the modified ID) to at least one remote computer device 26 via network 24, whereby the location ID_A received by the circuitry of the patient bed 20 is not transmitted by the circuitry 22 of bed 20. For example, if the location ID_A is 16 bits or 32 bits, or more, in length, the location ID_B may be shorter in length and yet still suitable for the purpose of indicating the room location, such as being 8 bits, thereby conserving transmission power and increasing bandwidth of network 24 by reducing the number of bits that are transmitted by bed 20 over the network 24.

According to this disclosure, the modified ID created by bed translation software 136 may also be in a more desirable format for receipt by other computer devices 26. For example, if location ID_A is a MAC address of locator unit

130, administrators of a healthcare facility may prefer to receive from bed 20 ASCII code of the room number for use in various other software programs on computer devices 26. Translation software 136, therefore, permits modified ID to be converted into the desired format. Computer device(s) 26, therefore, operate to associate the bed ID and modified ID in an association database and make no use of location ID_A.

Referring now to FIG. 14, another embodiment according to this disclosure includes a locator unit 130' that is mounted to a fixed location in a healthcare facility. Unit 130' has circuitry 132' with a transmitter 134' that is commanded by circuitry 132' to transmit a location ID. Circuitry 22 of bed 20 receives the location ID and has ID mutation software 140 that is stored in circuitry 22 and that mutates the location ID and the bed ID into to a single, unique mutated ID. Thereafter, circuitry 22 of bed 20 commands transmitter 28 to transmit the mutated ID to at least one remote computer device 26 via network 24, whereby the mutated ID transmitted from the patient bed 20 is neither the location ID nor the bed ID.

The mutation software 140, in some embodiments, uses a hash function, such as a cryptographic hash function, to mutate the location ID and the bed ID into the single, unique mutated ID. The one or more remote computer devices 26 then use ID decoding software 142 to correlate the mutated ID with the location ID and the bed ID. However, it should be appreciated that neither the location ID nor the bed ID were ever transmitted by the bed 20 to any device on the network 24.

To illustrate the method employed by software 140, consider the scenario in which location ID is in the form ROOM_ID_0001 and the bed ID is in the form BED_ID_0001. The software may add the location ID and the room ID and perform the hashing function by using software programming code such as SHA1

24

(ROOM_ID_0001+BED_ID_0001) and the resulting mutated ID, in hexadecimal format, is the following: 57e4f41a507079311acbb588d14cae4d564c7d43. While this example used the known SHA-1 hashing function, other known hashing functions may be employed in software 140, including the following: GOST, HAVAL, MD2, MD4, MD5, PANAMA, RadioGatun, RIPEMD, SHA-0, SHA-3, Tiger (2), and WHIRLPOOL.

Once the modified ID is created by the adding and hashing operation just described, the modified ID is transmitted off of the bed for receipt by one or more remote computer devices 26. The software 142 of each remote computer device 26 then uses a lookup table, in some embodiments, to correlate the received modified ID with the bed ID and room ID that created it. The lookup table includes the modified ID's and the associated bed ID and room ID for each possible combination of beds and rooms in a particular healthcare facility. An simple example of a lookup table for two beds that may be located in two different rooms is given as follows (and assumes a hashing function applied to the added room ID and bed ID as described above):

Bed ID	Room ID	Modified (e.g., added and hashed) ID
BED_ID_0001	ROOM_ID_0001	ffa6160a5ba73befd3f0cfdd5554613fad2094ed
BED_ID_0002	ROOM_ID_0001	6818ae262ae95541b03f5367829c1507e32ac595
BED_ID_0001	ROOM_ID_0002	bf2019c988268cd007ef7dcb0a280d1e75c8dd45
BED_ID_0002	ROOM_ID_0002	c1bf987848b483a8c6af9c4cf716466575db3dc7

Thus, if a bed with BED_ID_0001 as its bed ID is physically located in a room with ROOM_ID_0002 as its room ID, then bed 20 transmits via network 24 the modified ID bf2019c988268cd007ef7dcb0a280d1e75c8dd45 to the remote computer device 26 having software 142 and the software correlates the modified ID back to the room ID and bed ID that created it. However, neither the bed ID nor the room ID is transmitted by bed 20.

In an alternative embodiment, software 142 uses a list of all known bed ID's and a list of all known room ID's and the server computes the modified ID's (e.g., by adding and hashing) sequentially and compares each one to the received modified ID until a match is found, at which the point the bed ID and room ID that caused the match are known. This approach eliminates the need to store a large table of known combinations, but does potentially require a fair amount of computational power to perform the mutating operation sequentially.

In another contemplated embodiment, the bed only transmits a received or entered (e.g., via GUI 60) location ID along with other data such as bed status data. Thus, the bed ID is not transmitted off of the bed while the bed is in use. In such embodiments, the location ID is considered to be the bed ID while the bed is in the room associated with the room ID. In such embodiments, the bed may store in a database of circuitry 22 the room ID along with the start and end times at which the bed considered that particular room ID to be the bed ID. The start and end times include, for example, minutes, hours, day, month, and year. For many systems and software applications used in a healthcare environment, the end users are not interested in knowing the bed ID anyway. They are more interested in knowing which device status data goes with which patient. This can be accomplished in many instances by associating location ID, patient ID, and device status ID. In this regard, device status ID may include the patient's physiological data as measured by a particular

device. Manufacturers are more interested in knowing bed ID for service and maintenance purposes. Thus, at a later time, a service technician downloads the bed ID along with the rooms in which the bed was located in the past. Appropriate data analysis is made by the service technician after the download.

Referring now to FIG. 15, bed 20 optionally includes an indicator module 150 that mounts to a portion of bed 20 such as upper frame 152. In other embodiments, module 150 is mounted to some other portion of bed 20 such as base frame 154, one of endboards 156, or one of siderails 158. Indicator module 150 has a first light emitting diode (LED) 160 that is illuminated to indicate Wi-Fi signal strength between circuitry 22 (not shown in FIG. 15) of bed 20 (and/or circuitry 166 of module 150) and a wireless access point 124. In one embodiment, LED 160 is a three color LED (e.g., red, yellow, green) that is illuminated a particular color to indicate the relative signal strength. In some embodiments, wireless access point 124 operates to determine the signal strength of the communication link between it and circuitry 22 of bed 20 (or circuitry 166 of module 150) and, in other embodiments, circuitry 22 of bed 20 (or circuitry 166 of module 150) operates to determine the signal strength of the communication link between it and wireless access point 124.

Module 150 has a second LED 162 that is illuminated to indicate that a successful communication link has been established between circuitry 22 (not shown in FIG. 15) of bed 20 and one or more remote computer devices, such as devices 26a, 26b of FIG. 12, one or both of which may be considered a remote nurse call computer device. Module 150 has a third LED 164 that is illuminated to indicate that a successful bed-to-room association has been made at a remote computer device such as one or both of remote computer devices 26a or 26b of FIG. 12. In some embodiments, device 26a is a server of a real time location system (RTLS) and device 26b is a server of a nurse call system. Having third LED 164 included on module 150 is an improvement over known prior art beds which did not have any indicator relating to whether a successful bed-to-room association had been made. Alternatively or additionally, indicator 164 provides an indication of a successful bed-to-patient association, a successful room-to-patient association, and/or a successful bed-to-room-to patient association.

In one embodiment, circuitry 166 of module 150 includes a Model No. WB45NBT device available from Laird Technologies of Earth City, Mo. Details of the Model No. WB45NBT device can be found in *Laird Reference Manual, Laird WB45NBT*, Version 1.0, dated Aug. 20, 2013, which is hereby expressly incorporated by reference herein. Circuitry 166 of module 150 connects to circuitry 22 of bed 20 via a universal serial bus (USB) cable in some embodiments. In such embodiments, therefore, circuitry 22 and circuitry 166 each include a USB port. In other embodiments, circuitry 166 of module 22 and circuitry 22 of bed 20 communicate wirelessly. Circuitry 166 controls the illumination of LED's 160, 162, 164 via shift registers in some embodiments. Circuitry 166 includes a Wi-Fi antenna and/or a Bluetooth (BT) antenna in some embodiments. For example, a suitable antenna for either or both of these purposes is the Laird Model No. 95310 antenna. In some embodiments contemplated by this disclosure, circuitry 22 of bed 20 does not have wireless communication capability but instead relies on the wireless communication capability of circuitry 166 of module 150 to communicate bed data wirelessly to and from network 24 via wireless access point 124.

In some embodiments of the systems illustrated in FIGS. 12 and 15, the RTLS components are available from CenTrak, Inc. of Newtown, Pa. For example, in some embodiments, tag 118 is a CenTrak model no. IT-710 tag; RTLS location beacon or location unit 120 is a CenTrak model no. ITK-313 Monitor or a CenTrak model no. IT-323 Virtual Wall; and RTLS aggregator or transceiver 122 is a CenTrak model no. IT-103 Star. It should be appreciated, however, that RTLS components from other suppliers may be used in lieu of, or in addition to, the CenTrak components.

In alternative embodiments, RF triangulation is used to locate bed 20 in a healthcare facility. In such embodiments, tag 118, location unit 120 and transceiver 122 are omitted. Instead, multiple (typically three or more) Wi-Fi transceivers, such as wireless access points 124, receive wireless transmissions from bed 20 and then a remote computer device, such as one of servers 26a, 26b, analyzes signal strength and or time-of-flight information from the multiple wireless access points 124 to determine the location of bed 20. Once the location has been determined, bed 20 is notified wirelessly and indicator 164 of module 150 is illuminated.

Referring now to FIG. 16, a block diagram of a wireless bed-to-room association system similar to that of FIG. 12 but including a Wi-Fi module 150' is provided. In FIG. 16, Wi-Fi module 150' is similar to module 150 of FIG. 15. A wired connection 168, such as a USB cable, interconnects circuitry 22 and module 150'. It is within the scope of this disclosure for module 150' to be considered part of circuitry 22 but these are illustrated as separate blocks in FIG. 16 for ease of discussion. Thus, module 150' and its associated circuitry, like circuitry 166 of module 150, are integrated into the overall electrical system of bed 20 in some embodiments.

As shown diagrammatically in FIG. 16, a monitor ID 170 is transmitted from location unit 120, referred to in FIG. 16 as an RTLS location beacon, to an RTLS tag 118 mounted to bed 20. Monitor ID 170 is transmitted as a low frequency or infrared (IR) signal from beacon 120 as indicated by block 172. Thus, it is contemplated by this disclosure that only the tags 118 of beds in the same room or in close proximity to beacon 120 are able to receive monitor ID 170. After tag 118 has received monitor ID 170, tag 118 transmits a radio frequency (RF) signal, as indicated at block 174 in FIG. 16, that includes the monitor ID plus tag ID 176 for receipt by transceiver 122, which in FIG. 16 is referred to as an RTLS aggregator. The term "aggregator" is use because transceiver 122 will potentially receive RF signals from a multitude of beds 20 that are within its reception range. As indicated by diagrammatic arrow 178 in FIG. 16, the signals received by aggregator 122 are forwarded to remote computer device 26a which is referred to in FIG. 16 as an RTLS server. The monitor ID and Tag ID are paired to form a location association by RTLS server 26a as indicated by the text within arrow 178.

Still referring to FIG. 16, remote computer device 26b is coupled to RTLS server 26a via communication link 126. Device 26b is referred to as a bed data server in FIG. 16 but may just as well be referred to as a nurse call server. Bed data server 26b includes a database table 180 in which is stored, among other things, the location association information based on the monitor ID and tag ID pairing received from RTLS server 26a. Thus, one or both of servers 26a, 26b include RTLS Application Programming Interface (API) Integration software as indicated by the text within double headed arrow 126 of FIG. 16.

Wi-Fi module 150' of bed 20 sends a Wi-Fi signal, as indicated at block 182, that includes bed ID data 184. It

should be appreciated that bed **20** also transmits bed status data along with bed ID **184**. Bed status data includes bed frame data such as siderail position data, caster brake position data, lift system data, head of bed angle data, weigh scale system data, bed exit system data, motor lockout data, and the like; support surface data such as therapy mode data, maximum inflate data, turn assist data, and the like; and other data such as battery charge data, AC present/not present data, nurse call button data, and the like. For a more exhaustive list of bed status data that may be associated with bed **20**, see U.S. Patent Application Publication No. 2013/0135160 which is hereby incorporated by reference herein in its entirety to the extent not inconsistent with this disclosure which shall control as to any inconsistencies.

The bed status data and bed ID are received by server **26b** and are processed by bed data aggregator software **186** as indicated diagrammatically in FIG. **16**. Details of bed data aggregator software **186** can be found in U.S. Patent Application Publication No. 2012/0316892 which is hereby incorporated herein by reference herein in its entirety to the extent not inconsistent with this disclosure which shall control as to any inconsistencies. While FIG. **16** shows a single bed **20** communicating with server **26b**, it should be appreciated that a multitude of beds **20** communicate with server **26b**. Thus, the bed data aggregator software processes the bed status data and bed ID data from all of such beds.

Server **26a** and/or server **26b** stores information or has access to information that correlates the bed ID with the tag ID. Such information is entered into server **26a**, **26b** in connection with assigning tags **118** to the various beds **20** in some embodiments. Thus, the information correlating tag ID and bed ID is included in database table **180** in some embodiments. Furthermore, it will be appreciated that the monitor ID from each location beacon **120** corresponds to a particular location (e.g., room) of a healthcare facility. Accordingly, the bed status data that is transmitted with bed ID **184** is able to be associated with a particular location at which bed **20** is located due to the correlation of monitor ID with the tag ID of bed **20** and the correlation of the tag ID with the bed ID. These various correlated relationships are maintained in database **180** in some embodiments. The bed status data is also included in database **180** in some embodiments.

According to this disclosure, after the monitor ID, tag ID, and bed ID are correlated by server **26b**, a prospective or preliminary bed-to-room association is considered to exit. However, before the bed-to-room association is considered to be finalized, server **26b** determines whether a power plug **188** of power cord **190** of bed **20** is coupled into a receptacle **192** to receive AC power therefrom. The act of connecting plug **188** into receptacle **192** permits the inference to be drawn that bed **20** is likely to remain at the particular location for an extended period of time rather than simply being in transit or only temporarily at the location for a short period of time. If server **26b** determines that the bed status data indicates that bed **20** is receiving AC power from receptacle **192**, then location information **194** is transmitted to Wi-Fi module **150'** to indicate a successful or finalized bed-to-room association has been made.

Referring now to FIG. **17**, a flow chart of an algorithm **196** of a portion of the software executed by server **26b** of the system of FIG. **16** is shown. Block **198** of the algorithm states "Wireless 'Bed 1' Connects to Server," which means that server **26b** receives packets of data (e.g., bed ID **184** and bed status data) that have been communicated wirelessly from module **150'** of bed **20**. The packets are communicated to server **26b** via transceiver **122** and network **24** as

described previously in this disclosure. Thus, it should be appreciated that the so-called wireless packets are eventually communicated over various wired communication links (including fiber optic communication links in some embodiments) of the network infrastructure of a healthcare facility to reach server **26b**.

As indicated at block **200**, server **26b** looks for location ID associated with bed **20**. The location ID referenced in block **200** includes, for example, monitor ID **170** or a room number or other location name or number that correlates to monitor ID **170**. If at block **202**, server **26b** does not find a location ID that is associated with bed **20**, then the algorithm **196** loops back to block **200**. It will be appreciated that, if algorithm remains in the block **200**, **202** loop for a predetermined period of time or for a predetermined number of iterations, the software will exit from the loop and send an alarm message or return to some other portion of algorithm **196** or another algorithm.

If server **26b** finds the location ID for bed **20** at block **202**, server **26b** proceeds to block **204** to check the bed status message for "AC present" data which means that the plug **188** of power cord **190** of bed **20** is plugged into receptacle **192**. As indicated at block **206**, if server **26b** does not find AC present, then the algorithm **196** loops back to block **204**. It will be appreciated that, if algorithm remains in the block **204**, **206** loop for a predetermined period of time or for a predetermined number of iterations, the software will exit from the loop and send an alarm message or return to some other portion of algorithm **196** or another algorithm.

If server **26b** finds AC present at block **206**, server **26b** proceeds to block **208** and sends a message to bed **20**, including the Location or Room ID **194**, to indicate that bed **20** has been successfully located. Thereafter, bed **20** indicates a successful bed-to-room location by displaying the location ID (e.g., room name or number) on a graphical display screen of bed **20** or by otherwise indicating a successful bed-to-room location such as by illuminating indicator **164** of module **150** as discussed above in connection with FIG. **15**.

Referring now to FIG. **18** is a flow chart showing a disassociation algorithm **212** implemented by bed **20** and remote server **26b** of FIG. **16** in response to the bed **20** being disconnected from the AC power outlet or receptacle **192**. As indicated at block **214**, algorithm **212** begins in response to plug **188** of bed **20** being disconnected from receptacle **192**. After that occurs, bed **20** indicates no location such as, for example, by ceasing to display the room name or number on a graphical display screen of bed **20** or by turning off indicator **164** of module **150**. Algorithm **212** then proceeds to block **218** at which bed **20** sends a message to server **26b** indicating that AC is no longer present due to the unplugging of plug **188** from receptacle **192**. After server **26b** receives that message from bed **20**, server **26b** disassociates bed **20** from the last location as indicated at block **220** and proceeds to indicate no location for bed **20** as indicated at block **222**. In some embodiments, this involves removing data from table **180**. For example, the bed ID and bed status data may be maintained in table **180** but the monitor ID, tag ID and/or location ID (or other location information such as room name or room number) is removed and, if desired, replace with the string "no location." Alternatively, the monitor ID, tag ID and/or location ID (or other location information) is maintained in the table **180** and the bed ID and/or bed status data is removed from table **180**.

Referring now to FIG. **19** a patient-to-bed association system includes a wireless heart rate monitor **224** that includes circuitry **226** configured to send data, including the

patient's medical record number (MRN), wirelessly to circuitry of bed 20. In FIG. 19, the circuitry of bed is omitted but suffice it to say that the circuitry of bed 20 is discussed elsewhere herein in connection with each of the other embodiments in which bed 20 has wireless communication capability. As indicated by diagrammatic arrow 228 in FIG. 19, bed 20 is configured to transmit the patient's MRN and bed ID data wirelessly for used by one or more remote computer devices (e.g., servers 26a, 26b) to associate the patient to the bed 20. In some embodiments, heart rate monitor 224 also sends heart rate data to bed 20 for display on a graphical display screen of bed 20 or for wireless transmission to remote computer devices such as servers 26a, 26b and/or to one or more computer devices of an EMR system.

Circuitry 226 of heart rate monitor 224 is programmable with the patient's MRN. For example, such programming may occur upon admittance of the patient to a healthcare facility. In some embodiments, circuitry 226 includes a Bluetooth module for communication of wireless data via the Bluetooth protocol. A suitable heart rate monitor is the Wahoo Blue TICKR monitor available from Wahoo Fitness of Atlanta, Ga. In the illustrative example of FIG. 19, monitor 224 is coupled to the patient's arm via an arm band 230. In other embodiments, monitor 224 is coupled to the patient by a chest band that is similar to arm band 230, but larger to fit around the circumference of the patient's chest. In some embodiments, arm band 224 is adjustable and so is expandable so as to be usable as a chest band.

Alternatively or additionally, monitor ID data of heart rate monitor 224 is mapped or correlated with the patient's ID data in a database, such as in a database of RTLS server 26a or in database table 180 of server 26b or some other server such an ADT server. The monitor ID data is transmitted wirelessly from monitor 224 to bed 20 and then sent wireless from the bed 20 along with the bed ID data as indicated diagrammatically by arrow 228 in FIG. 19. Regardless of whether the patient's MRN is used or monitor ID data is used, a patient-to-bed association and therefore, a patient-to-bed-to-room association is made within database table 180 of server 26b in some embodiments. The capability to pair or otherwise association a patient with medical equipment or than bed 20 using heart rate monitor 224 in a similar manner is also contemplated by this disclosure. This is possible as long as the other medical equipment has the same or similar wireless communication capability as bed 20.

Referring now to FIG. 20, another bed data system is shown diagrammatically in which bed 20 is equipped with a first Bluetooth (BT) module 232 and optionally, in some embodiments, a second BT module 234. Modules 232, 234 communicate with a wall BT module 236 for transmission of bed data, including bed status data and bed ID data, after a BT pairing operation is conducted based on transmission of bed BT module ID data via a transponder 238 carried by a plug of a power cord 240 of bed 20 as indicated by diagrammatic block 242. It is contemplated by this disclosure that modules 232, 234, 236 are Class 2 Bluetooth devices that have a theoretical communication range of up to 33 feet (10 meters) but, in practice, have a communication range on the order of 15-20 feet. This is not to say that in other embodiments, Class 1 Bluetooth devices having a theoretical range of 329 feet (100 meters) or Class 3 Bluetooth devices having a theoretical range of 3.3 feet (1 meter) could not be used in lieu of modules 232, 234, 236. Furthermore, modules using other types of communication

technology (e.g., ZigBee, Wi-Fi) are also within the scope of this disclosure for use as alternatives to modules 232, 234, 236.

By using modules 232, 234, 236, the traditional bed status or nurse call cable (e.g., a 37-pin connector cable) between bed 20 and a nurse call module 244 is eliminated. Thus, the power cord 240 is the only cord that connects to, and disconnects from, an associated receptacle. The bed data is communicated wirelessly from one or both of modules 232, 234 to module 236. In the illustrative example of FIG. 20, it is assumed that a nurse call system 246 having one or more nurse call modules 244 in each room is already installed in a healthcare facility. The nurse call modules 244 each are communicatively coupled to a nurse call server 246 as illustrated diagrammatically in FIG. 20 with double headed arrow 247. Thus, to convert the wireless data received by module 236 from either or both of modules 232, 234 into wired data that can be fed to the existing nurse call module 244, a communication board or circuit 248 is provided. Communication circuit 248 communicates with module 236 as indicated by double headed arrow 250. A 37-pin connector cable 252 interconnects communication circuit 248 and nurse call module 244 as indicated by diagrammatic block 254. Data received at nurse call module 244 is communicated to nurse call server 246.

In the illustrative embodiment, wall Bluetooth module 236 communicates with modules 232, 234 via radio frequency (RF) signals according to the Bluetooth protocol which operates on an unlicensed 2.4 gigahertz (GHz) band which is also shared with Wi-Fi and other protocols. To be more specific, the Bluetooth protocol implements an adaptive frequency hopping (AFH) methodology to transmit at any of 79 hopping channels that are 1 megahertz (MHz) apart between 2.4 GHz and 2.4835 GHz. Thus, in addition to receiving wireless signals from modules 232, 234 of bed 20, it is foreseeable that wall BT module 236 will be within the reception range of other devices, including other beds 20, and receive the wireless signals transmitted by those other devices. So, in order to pair module 236 with one or both of modules 232, 234, a loop antenna 256 is provided to read signals sent from transponder 23 as indicated diagrammatically at block 258 in FIG. 20. The signals from transponder 23 are encoded with a first module ID of first module 232 and, if present, a second module ID of second module 234.

If module 232 is the only module on bed 20, then in response to power cord 240 being plugged in, loop antenna 256 is powered up by communication circuit 248 and reads the first module ID from transponder 238 to communication circuit 248. Communication circuit then provides the first module ID to wall BT module 236. In some embodiments, the first module ID corresponds to a unique 48 bit Bluetooth device address (aka the MAC address) of module 232. The first 24 bits of this address represent the manufacturer of the Bluetooth circuitry of module 232 and the remaining 24 bits are unique for each Bluetooth device assigned by the manufacturer. However, any unique module ID would suffice. After receiving the first module ID, wall BT module 236 then operates to accept wireless transmissions from only module 232 and to ignore all other wireless transmissions. In this regard, module 236 accepts wireless transmission packets that contain the first module ID. This is sometimes referred to as an Out of Band (OOB) pair between modules 232, 236.

The transmission packets sent between modules 232, 236 include both audio and data packets in some embodiments. For example, Bluetooth technology is rated for 3 Mega bits

per second (Mbps) transmission speed, but in practice the speed is about 2.1 Mbps, which is fast enough to permit audio and data packets to be sent. The delay in the audio signal using Bluetooth technology is about 50 to about 80 milliseconds (ms) which is less than the 100 ms delay required to synchronize television video and audio. Thus, modules 232, 236 of the system in FIG. 20 are an improvement over prior art bed data systems in which transmission of audio data was not possible.

If power cord 240 is unplugged, loop antenna 256 no longer provides the first module ID to communication circuit 248 and communication circuit 248 notifies wall BT module 236 to break its pairing with module 232 of bed 20. During the communication between module 232, 236, module 236 operates as a “master” module such as by controlling the frequency hopping channels over which communications with module 232 occur, and module 232, therefore, operates as a “slave.”

If modules 232, 234 are both present on bed 20, then in response to power cord 240 being plugged in, loop antenna 256 is powered up by communication circuit 248 and reads the first module ID and the second module ID from transponder 238 to communication circuit 248. Communication circuit then provides the first module ID and the second module ID to wall BT module 236. Module 236, acting as a “master,” assesses the signal strength of the communications from modules 232, 234 and chooses to communicate with the “slave” (i.e., one or the other of modules 232, 234) that has lower RF interference based on received signal strength indicator (rssi) and channel map. If communication with the chosen slave is lost at any time after the master-slave relationship between module 236 and one of modules 232, 234 is established, module 236 jumps or switches the communication over to the other of modules 232, 234 if the RF interference with the other of modules 232, 234 is acceptable. In some embodiments, if the master module 236 is unable to communicate with both slave modules 232, 234, then at least one of modules 232, 234, 236 triggers an audible and/or visual alarm.

In the illustrative embodiment, module 232 is on one side of bed 20 and module 234 is on the other side of bed 20. For example, module 232 is coupled to a right siderail of bed 20 and module 234 is coupled to a left siderail of bed 20 in some embodiments. It is contemplated by this disclosure that bed 20 may include an additional Wi-Fi module such as, for example, modules 150, 150' discussed above. It is preferable to place the Wi-Fi module on bed 20 as far from modules 232, 234 as possible since Wi-Fi operates in the same frequency band as Bluetooth. However, placing the additional Wi-Fi module at the head end of bed 20 between modules 232, 234 at the sides of bed 20 is sufficient. It is contemplated by this disclosure that the first and second BT modules 232, 234 communicate in different time slots than the additional Wi-Fi module communicates. Thus, when either of the modules 232, 234 are turned on, the additional Wi-Fi module is turned off and vice versa. Thus, the time slots of transmission are non-overlapping time slots.

Referring now to FIG. 21, the scenario is illustrated in which a prior art bed 20' that lacks any wireless modules, such as modules 232, 234, is still able to be used with the system of FIG. 20. In this situation, bed 20' has a power cord 240' that does not have any transponder as indicated at diagrammatic block 242'. Instead, a traditional connector nurse call connector cable 260 is provided to provide a wired communication link between bed 20' and nurse call module 244. In the FIG. 21 example, it is contemplated that nurse call module 244 has only one nurse call cable connection

port, such as a single 37-pin connection port. Thus, connector cable 252 is shown in FIG. 21 as being unplugged from the nurse call module 244 so that connector cable 260 can be plugged into the nurse call module 244. In some embodiments, nurse call module 244 is a Bed Interface Unit (BIU) that is marketed by Hill-Rom Company, Inc. of Batesville, Ind. In the FIG. 21 example, module 236, communication circuit 248, and loop antenna 256 are dormant, at least with regard to communication of bed data from bed 20' to and from nurse call server 246.

Referring now to FIG. 22, the scenario is illustrated in which a nurse call module 244' has two nurse call cable connection ports, such as having two 37-pin cable connection ports. An example of such a nurse call module 244' is a Network Interface Unit (NIU) which is indicated at diagrammatic block 262 in FIG. 22 and which is marketed by Hill-Rom Company, Inc. of Batesville, Ind. So, in the FIG. 22 example, cable 252 remains plugged into one of the connection ports of nurse communication module 244' even when the prior art bed 20' has its nurse call cable 260 plugged into the other of the connection ports of nurse call module 244'. In this situation, circuitry in nurse call module 244' operates so that the wired communication link between bed 20' and nurse call module 244' via cable 260 takes priority over the wired communication link between communication circuit 248 and nurse call module 244' via cable 252. In some embodiments, one of the connection ports of module 244' is a male 37-pin connector and the other of the connection ports of module 244' is a female 37-pin connector. The mating connectors at the ends of cables 252, 260 are fashioned accordingly.

Referring now to FIG. 23, loop antenna 256 of FIGS. 20-22 is shown situated beside a receptacle 264 of a duplex AC outlet 266 as indicated with diagrammatic block 268. For example, antenna 256 is mounted to a back surface of a duplex cover plate 270 adjacent the aperture 272 in cover plate 270 that receives receptacle 264. A first AC power cord 240a has its transponder 238 embodied as an RFID tag that is molded into a plug body 272 as indicated at diagrammatic block 274. Transponder 238 in plug body 272 is located closely behind a front surface 276 from which power prongs 278, 279 and ground prong 280 extend. When prongs 278, 279, 280 are received in a receptacle 265 of duplex AC outlet 266, transponder 238 of plug body 272 is sufficiently close to loop antenna 256 for wireless communication to be established therebetween. Of course, prongs 278, 279, 280 may also be received in receptacle 264, if desired, and antenna 256 and transponder 238 will communicate just as well. In the illustrative example, cord 240a and plug body 272 meet NEMA 5-15 hospital grade requirements.

A second AC power cord 240b has its transponder 238 embodied as an RFID tag included in a label 282 as indicated at diagrammatic block 284 in FIG. 23. Label 282 attaches to cord 240b at a position spaced from, but adjacent to, a plug body 286. Power prongs 287, 288 and a ground prong 289 extend from plug body 286. When prongs 287, 288, 289 are received in receptacle 264 (or receptacle 265, if desired) of duplex outlet 266, transponder 238 of label 282 is sufficiently close to loop antenna 256 for wireless communication to be established therebetween.

Active and passive transponders 238 (e.g., RFID tags) are contemplated by this disclosure. For example, transponder 238 of label 282 is a passive transponder whereas transponder 238 of plug body 272 is an active transponder that is powered by a 5 Volt (V) or 3.3 V power supply of bed 20. As shown in FIG. 25, power cord 240a contains AC power conductors 290, 292, a ground conductor 294, and DC

power/data conductors **296, 298**. Conductors **290, 292, 294** are coupled to prongs **278, 279, 280**, respectively, and conductors **296, 298** are coupled to transponder **238** in plug body **272**. Thus, conductors **296, 298** provided the power to transponder **238** and are also usable as data lines to program the first and second module ID's into memory of transponder **238**.

In some embodiments, transponder **238** is an RFID tag having an EEPROM which is programmed by bed circuitry **22**, such as by using a multipoint control unit (MCU), via a serial peripheral interface (SPI) protocol or Inter-Integrated Circuit (I2C) protocol. For the passive transponder **238**, the first and second module ID's are written to memory wirelessly. In some embodiments contemplated by this disclosure, transponders **238** are programmed in an active mode, such as via conductors **296, 298**, and then operate in a passive mode when loop antenna **256** is reading the module ID's from the transponder **238**. In such embodiments, loop antenna **256** is energized by communication circuit **248** and transfers energy to transponder **238** that is used by the transponder to transmit the first and second module ID's for reception by antenna **256**.

Referring now to FIG. **24**, AC power cord **240a** carries a first RFID component **300** in plug body **272** and a receptacle module **302** has a housing **304** that carries a second RFID component **306**. Module **302** has an AC receptacle **308** at a front face **310** thereof. In some embodiments, module **302** plugs into an existing AC outlet and so power and ground prongs (not shown) extend from a back of housing **304** in such embodiments. In other embodiments, receptacle is wired directly to the power grid of the corresponding healthcare facility. Module **302** also has a light-up ring **312** that is provided at front face **310** and that circumscribes or encompasses receptacle **312**. Light-up ring **312** is illuminated when a successful bed-to-room association has been made.

In a first scenario for determining a successful bed-to-room association, RFID component **306** includes a reader that receives bed ID data from RFID component **300** when power cord **240a** is plugged in with prongs **278, 279, 280** being received by receptacle **308** of module **302**. After RFID component **306** receives the bed ID data from RFID component **300**, module **302** sends room ID data to the circuitry **22** of the bed **20** that is designated with the bed ID data using wireless transmission circuitry included in module **302**. In some embodiments, the wireless communication circuitry of module **302** operates according to the Bluetooth protocol. In such embodiments, bed **20** includes Bluetooth circuitry. Bed **20** receives the room ID data and then transmits the bed ID data and the room ID data using a Wi-Fi transmitter of circuitry **22**. Bed **20** also transmits a Bluetooth message back to the circuitry of module **302** to confirm the bed-to-room association. In response to that message, module illuminates light-up ring **312**. Ring **312** is illuminated green in some embodiments.

In a second scenario for determining a successful bed-to-room association, RFID component **306** includes a passive RFID tag and RFID component **300** comprises a reader that receives power from conductors **296, 298** of cord **240a**. RFID component **300** senses RFID component **306** when cord **240a** is plugged into module **302** and reads room ID data that is encoded in RFID component **306**. RFID component **300** then sends the room ID data to circuitry **22** of bed **20** via wired connection, such as one or both of conductors **296, 298**. Bed **20** then transmits the bed ID data and the room ID data using a Wi-Fi transmitter of circuitry **22**. In this scenario, module **302** receives a Wi-Fi signal or

other wireless signal once a successful bed-to-room association is made (either at bed **20** or at a remote computer device, such as servers **26a, 26b**) and the circuitry of module **302** turns on the light-up ring **312** to indicate the successful bed-to-room association.

Referring now to FIG. **26**, another bed-to-room association system according to this disclosure is shown in which bed **20** has wireless transceiver, such as an illustrative Bluetooth transceiver **150"**, coupled to circuitry **22** and operable to establish wireless communications with circuitry **314** of a handheld pillow speaker unit **320** as indicated by diagrammatic dashed arrow **316**. In this embodiment, the pillow speaker unit **320** acts as a communication intermediary between the bed **20** and a nurse call system **322** as well as one or more other remote computer devices **324**. Bed data, including bed status data and bed ID data, is communicated to unit **320** wirelessly from bed **20** for reception by an antenna or transceiver **315** of circuitry **314** and, in turn, circuitry **314** of unit **320** sends the bed data to nurse call system **322** along with pillow speaker unit ID data. A computer device of nurse call system **322** and/or one of the other computer devices **324** includes a database that correlates the pillow speaker unit ID data with a patient room **326** in which unit **320**, and therefore, bed **20** is located.

Pillow speaker unit **320** is coupled via a wired power and data connection to a nurse call interface **330** as indicated by diagrammatic double headed arrow **328**. Nurse call interface **330** is coupled to nurse call system **322** as indicated by diagrammatic double headed arrow **332**. Nurse call interface **330** is also coupled to a television (TV) **334**, room lights **336**, and window shades **338** as indicated by diagrammatic arrows **340, 342, 344**, respectively. Pillow speaker unit **320** has user inputs **350** that are used to control functions of TV **334**, lights **336**, shades **338**, and bed **20**. Bed **20** has user inputs **352** that are also used to control functions of TV **334**, lights **336**, shades **338**, and bed **20**. Thus, when user inputs **350** of unit **320** are used to control bed **20**, control signals from unit **320** are communicated to transceiver **150"** wirelessly from circuitry **314** of unit **320**. Similarly, when user inputs **352** of bed **20** are used to control TV **334, 336, 338**, control signals from bed **20** are communicated from transceiver **150"** wirelessly to circuitry **314** of unit **320**. A pairing operation, such as the pairing operation described above in connection with FIG. **20**, takes place between the circuitry **314** of unit **320** and the circuitry of bed **20** so that other, unrelated wireless transmissions are ignored by unit **320** and bed **20**.

Referring now to FIG. **27**, a first embodiment of handheld pillow speaker unit **320** is shown in which a housing **321** carries a set of manual buttons **350a** and a graphical user interface (GUI) **350b** having electronic touchscreen buttons **354**. The manual buttons **350a** are located beneath the GUI **350b** in the illustrative example. Known prior art pillow speaker units only have manual buttons. Thus, by equipping unit **320** with GUI **350b**, unit **320** is able to have more sophisticated functionality than known pillow speaker units. However, pillow speaker unit **320** includes a manual nurse call button **356** which is pressed to send a general nurse call signal to nurse call system **322** in order to contact or summon an assigned caregiver. Others of the manual buttons are used to place telephone calls, to control TV **334**, to control a radio, and to control room lights **336** and shades **338** in some embodiments.

In some embodiments, the touchscreen buttons **354** of GUI **350b** have the functionality described in U.S. application Ser. No. 14/177,851, which was filed Feb. 11, 2014, which is titled "Workflow Canvas for Clinical Applica-

35

tions,” and which is hereby incorporated by reference herein to the extent not inconsistent with the present disclosure which shall control as to any inconsistencies. In general, each button **354** is selected to send a specific message to an assigned caregiver. Such messages, for example, indicate that the patient needs to go to the bathroom, that the patient wants water, that the patient is in pain, that there is a problem with an intravenous (IV) pump or liquid, that there is a problem with a catheter, or that there is a problem with other equipment, such as bed **20**. This list of messages is not intended to be exhaustive but merely to give a few examples. GUI **350b** also permits a user to navigate to screens for controlling bed functions in some embodiments.

Referring now to FIG. **28**, is a second embodiment of a handheld pillow speaker unit **320'** is shown in which a housing **321'** carries a reduced set of manual buttons **350a'** but still has GUI **350b** with electronic touchscreen buttons **354**. The reduced set of manual buttons includes manual nurse call button **356** beneath the GUI **350b**, a first on/off button **358** for control of a first light, and a second on/off button **360** for control of a second light. For example, the first light is one of room lights **336** and the second light is a reading light of bed **20** in some embodiments.

It will be appreciated that units **320**, **320'** of FIGS. **27** and **28** have traditional manual buttons **350a**, **350b** that older patients may be more comfortable using and also have GUI **350b** that is similar to modern day smart phones that younger patients may be more comfortable using. However, because units **320**, **320'** are tethered to nurse call interface **330** by wired connection **328**, units **320**, **320'** will not become lost or misplaced by patients as may tend to occur if units **320**, **320'** were wireless units. The enhanced functionality afforded to units **320**, **320'** by GUI **350b** allows for a better patient experience due to more effective communications between the patient and the caregiving staff of the healthcare facility.

Each of the embodiments disclosed herein can have features of one or more of each of the other embodiments. For example, the patient-to-bed association system of FIG. **19** in which a patient wears a device that transmits data that corresponds to patient ID can be used in combination with the various embodiments of FIGS. **1-18** and **20-28**. Furthermore, it is contemplated that a system can employ different bed-to-room association embodiments in different patient rooms. Thus, one room of a healthcare facility may have the embodiment of FIG. **1** or **2** (location data encoded in light), another room in the healthcare facility may have the embodiment of FIG. **3** or **4** (bar code array), another room in the healthcare facility may have the embodiment of FIGS. **5-10** (manual location entry), and so on. Thus, a system employing, at the same time, each and every embodiment disclosed herein is within the scope of this disclosure.

Although certain illustrative embodiments have been described in detail above, variations and modifications exist within the scope and spirit of this disclosure as described and as defined in the following claims.

The invention claimed is:

1. A system for associating a bed to a room of a healthcare facility, the system comprising
 a locator unit that is fixed in place in the room and that transmits a location ID,
 a patient bed having first circuitry that has a first ID and that receives the location ID, the patient bed having second circuitry that is independent of the first circuitry, the second circuitry being configured to transmit a bed ID and bed status data,

36

a first transceiver spaced from the locator unit and spaced from the patient bed, the first transceiver receiving the first ID and location ID transmitted by the first circuitry, a second transceiver that is spaced from and independent of the first transceiver, the second transceiver receiving the bed ID and the bed status data transmitted by the second circuitry,

a first remote computer device receiving the location ID and first ID transmitted to the first remote computer device by the first transceiver, and

a second remote computer device that receives the bed ID and the bed status data which is transmitted to the second computer device by the second transceiver, wherein the first and second remote computer devices cooperate to associate the location ID and the bed status data with the bed ID, wherein the patient bed includes an indicator coupled to the second circuitry and that is signaled by the second circuitry to provide an indication that a successful bed-to-room association has been made.

2. The system of claim **1**, wherein the first circuitry is included as part of a tag that attaches to an exterior surface of the patient bed.

3. The system of claim **1**, wherein the first circuitry transmits the first ID and the location ID using a first wireless transmission technology, the second circuitry transmits the bed ID and the bed status data using a second wireless transmission technology, and the first wireless transmission technology differs from the second wireless transmission technology.

4. The system of claim **3**, wherein the first wireless transmission technology comprises one of infrared technology, radio frequency technology, and ultrasonic technology and the second wireless transmission technology comprises a different one of infrared technology, radio frequency technology, and ultrasonic technology.

5. The system of claim **1**, wherein the indicator is turned on in response to the successful bed-to-room association being made and the indicator being turned off in the absence of the successful bed-to-room association.

6. The system of claim **1**, wherein the indicator is illuminated a first color in response to the successful bed-to-room association being made and the indicator being illuminated a second color in the absence of the successful bed-to-room association.

7. The system of claim **1**, wherein the indication that the successful bed-to-room association has been made is communicated to the second circuitry from the first remote computer device or the second remote computer device.

8. The system of claim **1**, wherein the patient bed includes at least one other indicator that includes a communication indicator to indicate that a successful communication link has been established with the second remote computer device via the second transceiver.

9. The system of claim **1**, wherein the patient bed includes at least one other indicator that includes an alarm monitor indicator to indicate that one or more conditions of the patient bed have been selected using the second remote computer for monitoring of alarm conditions.

10. The system of claim **1**, wherein the patient bed includes at least one other indicator that includes a signal strength indicator that indicates a strength of a wireless communication link with the second transceiver.

11. The system of claim **1**, wherein the second circuitry is only notified of the successful bed-to-room association if the

bed status data includes information indicating that a power cord of the patient bed is plugged into a power outlet in the room.

12. The system of claim 1, wherein the patient bed includes a graphical display that is coupled to the second circuitry and that is signaled by the second circuitry to display location information on the graphical display as an indication that a successful bed-to-room association has been made.

13. The system of claim 1, wherein the first circuitry receives the location ID via infrared (IR) communication.

14. The system of claim 1, wherein the first circuitry transmits the location ID and the first ID using radio frequency (RF) communication.

15. The system of claim 1, wherein the second circuitry communicates wireless using Wi-Fi communication.

16. The system of claim 1, further comprising a second patient bed and association means for associating the second patient bed to a second room of the healthcare facility.

17. The system of claim 13, wherein the association means comprises at least one or more of the following:

(i) a light source that emits visible light having a signature that is unique to a location of the healthcare facility;

(ii) an array of redundant bar codes and a bar code reader that is coupled to the second patient bed and that reads at least one of the redundant bar codes in the array;

(iii) a graphical user interface that is coupled to the second patient bed and that displays at least one user interface screen that is used by a caregiver to manually enter location data indicative of a location in a healthcare facility occupied by the second patient bed;

(iv) third circuitry coupled to the second patient bed and having stored therein ID translation software, the third circuitry receiving a second room location ID in a first format and, in accordance with the ID translation software, converting the second room location ID to a modified ID having a second format different than the first format, the third circuitry transmitting the modified ID;

(v) fourth circuitry coupled to the second patient bed and having stored therein ID mutation software, the fourth

circuitry receiving the second location ID and, in accordance with the ID mutation software, mutating the second location ID and a second bed ID of the second bed into a mutated ID, the mutated ID being a single unique ID, the fourth circuitry transmitting the mutated ID;

(vi) at least one bed Bluetooth (BT) module coupled to the second patient bed and in communication with a wall BT module for transmission of bed data after a BT pairing operation is conducted based on transmission of bed BT module ID data via a transponder carried by a plug of a power cord of the second patient bed;

(vii) a power cord of the second patient bed carrying a first RFID component, and a receptacle module carrying a second RFID component, the receptacle module having a receptacle into which the power cord plugs to receive power and to bring the first and second RFID components into communicative proximity, the receptacle module having an indicator that is activated in response to successful communication being established between the first and second RFID components.

18. The system of claim 1, further comprising an apparatus for communicating with a nurse call system of the healthcare facility, the apparatus comprising a second patient bed configured for wireless communication of second bed identification (ID) data and second bed status data, and a handheld pillow speaker unit having a pillow speaker transceiver in wireless communication with the second patient bed, the pillow speaker unit being in hardwired communication with the nurse call system, wherein the pillow speaker unit serves as a communication intermediary between the second patient bed and the nurse call system.

19. The system of claim 1, further comprising a pillow speaker unit to communicate with a nurse call system of the healthcare facility, the pillow speaker unit comprising a handheld housing, a set of manual buttons accessible on the housing, and a touchscreen graphical display that displays electronic buttons, at least one of the manual buttons and at least one of the electronic buttons being usable to send a respective signal to the nurse call system.

* * * * *