



US011083439B2

(12) **United States Patent**
Chan et al.

(10) **Patent No.:** **US 11,083,439 B2**
(45) **Date of Patent:** **Aug. 10, 2021**

(54) **COOLING UNIT FOR AN ULTRASOUND IMAGING APPARATUS, AND RELATED ULTRASOUND SYSTEMS**

(71) Applicant: **Clarius Mobile Health Corp.**, Burnaby (CA)

(72) Inventors: **Kwun-Keat Chan**, Vancouver (CA); **Binda Zhang**, Surrey (CA); **Daniel Rahardja**, Burnaby (CA)

(73) Assignee: **Clarius Mobile Health Corp.**, Vancouver (CA)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 447 days.

(21) Appl. No.: **15/614,488**

(22) Filed: **Jun. 5, 2017**

(65) **Prior Publication Data**

US 2018/0344294 A1 Dec. 6, 2018

(51) **Int. Cl.**
A61B 8/00 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 8/546** (2013.01); **A61B 8/4411** (2013.01); **A61B 8/44** (2013.01); **A61B 8/4472** (2013.01)

(58) **Field of Classification Search**

None
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,560,362 A * 10/1996 Sliwa, Jr. A61B 8/546
600/439
5,961,465 A * 10/1999 Kelly, Jr. A61B 8/546
600/459

6,362,958 B1 3/2002 Yu et al.
6,542,846 B1 4/2003 Miller et al.
6,709,392 B1 3/2004 Salgo et al.
6,795,314 B1 9/2004 Arbogast et al.
6,980,419 B2 12/2005 Smith et al.
7,948,754 B2 5/2011 Huang
7,998,072 B2 8/2011 Phelps et al.
8,143,898 B1 * 3/2012 Markoff A61B 8/4444
324/522

(Continued)

FOREIGN PATENT DOCUMENTS

JP 2010088610 A * 4/2010

OTHER PUBLICATIONS

International Search Report and Written Opinion of the International Searching Authority for corresponding PCT International Application No. PCT/CA2018/050632 dated May 30, 2018.

Primary Examiner — Angela M Hoffa


Assistant Examiner — Younhee Choi

(74) *Attorney, Agent, or Firm* — Julian Ho

(57) **ABSTRACT**

Cooling units for an ultrasound imaging apparatus, and related ultrasound systems are described. The ultrasound imaging systems may include an ultrasound imaging apparatus operable to acquire ultrasound image data; and a cooling unit configured to detachably couple to the ultrasound imaging apparatus. The cooling unit may be cordless and include an active cooling element for removing heat from the ultrasound imaging apparatus. The ultrasound imaging apparatus may have a sensor to determine when the cooling unit is attached. The cooling unit may have an identity interface, and the ultrasound imaging apparatus may use the identity interface to determine whether the cooling unit is compatible.

10 Claims, 7 Drawing Sheets

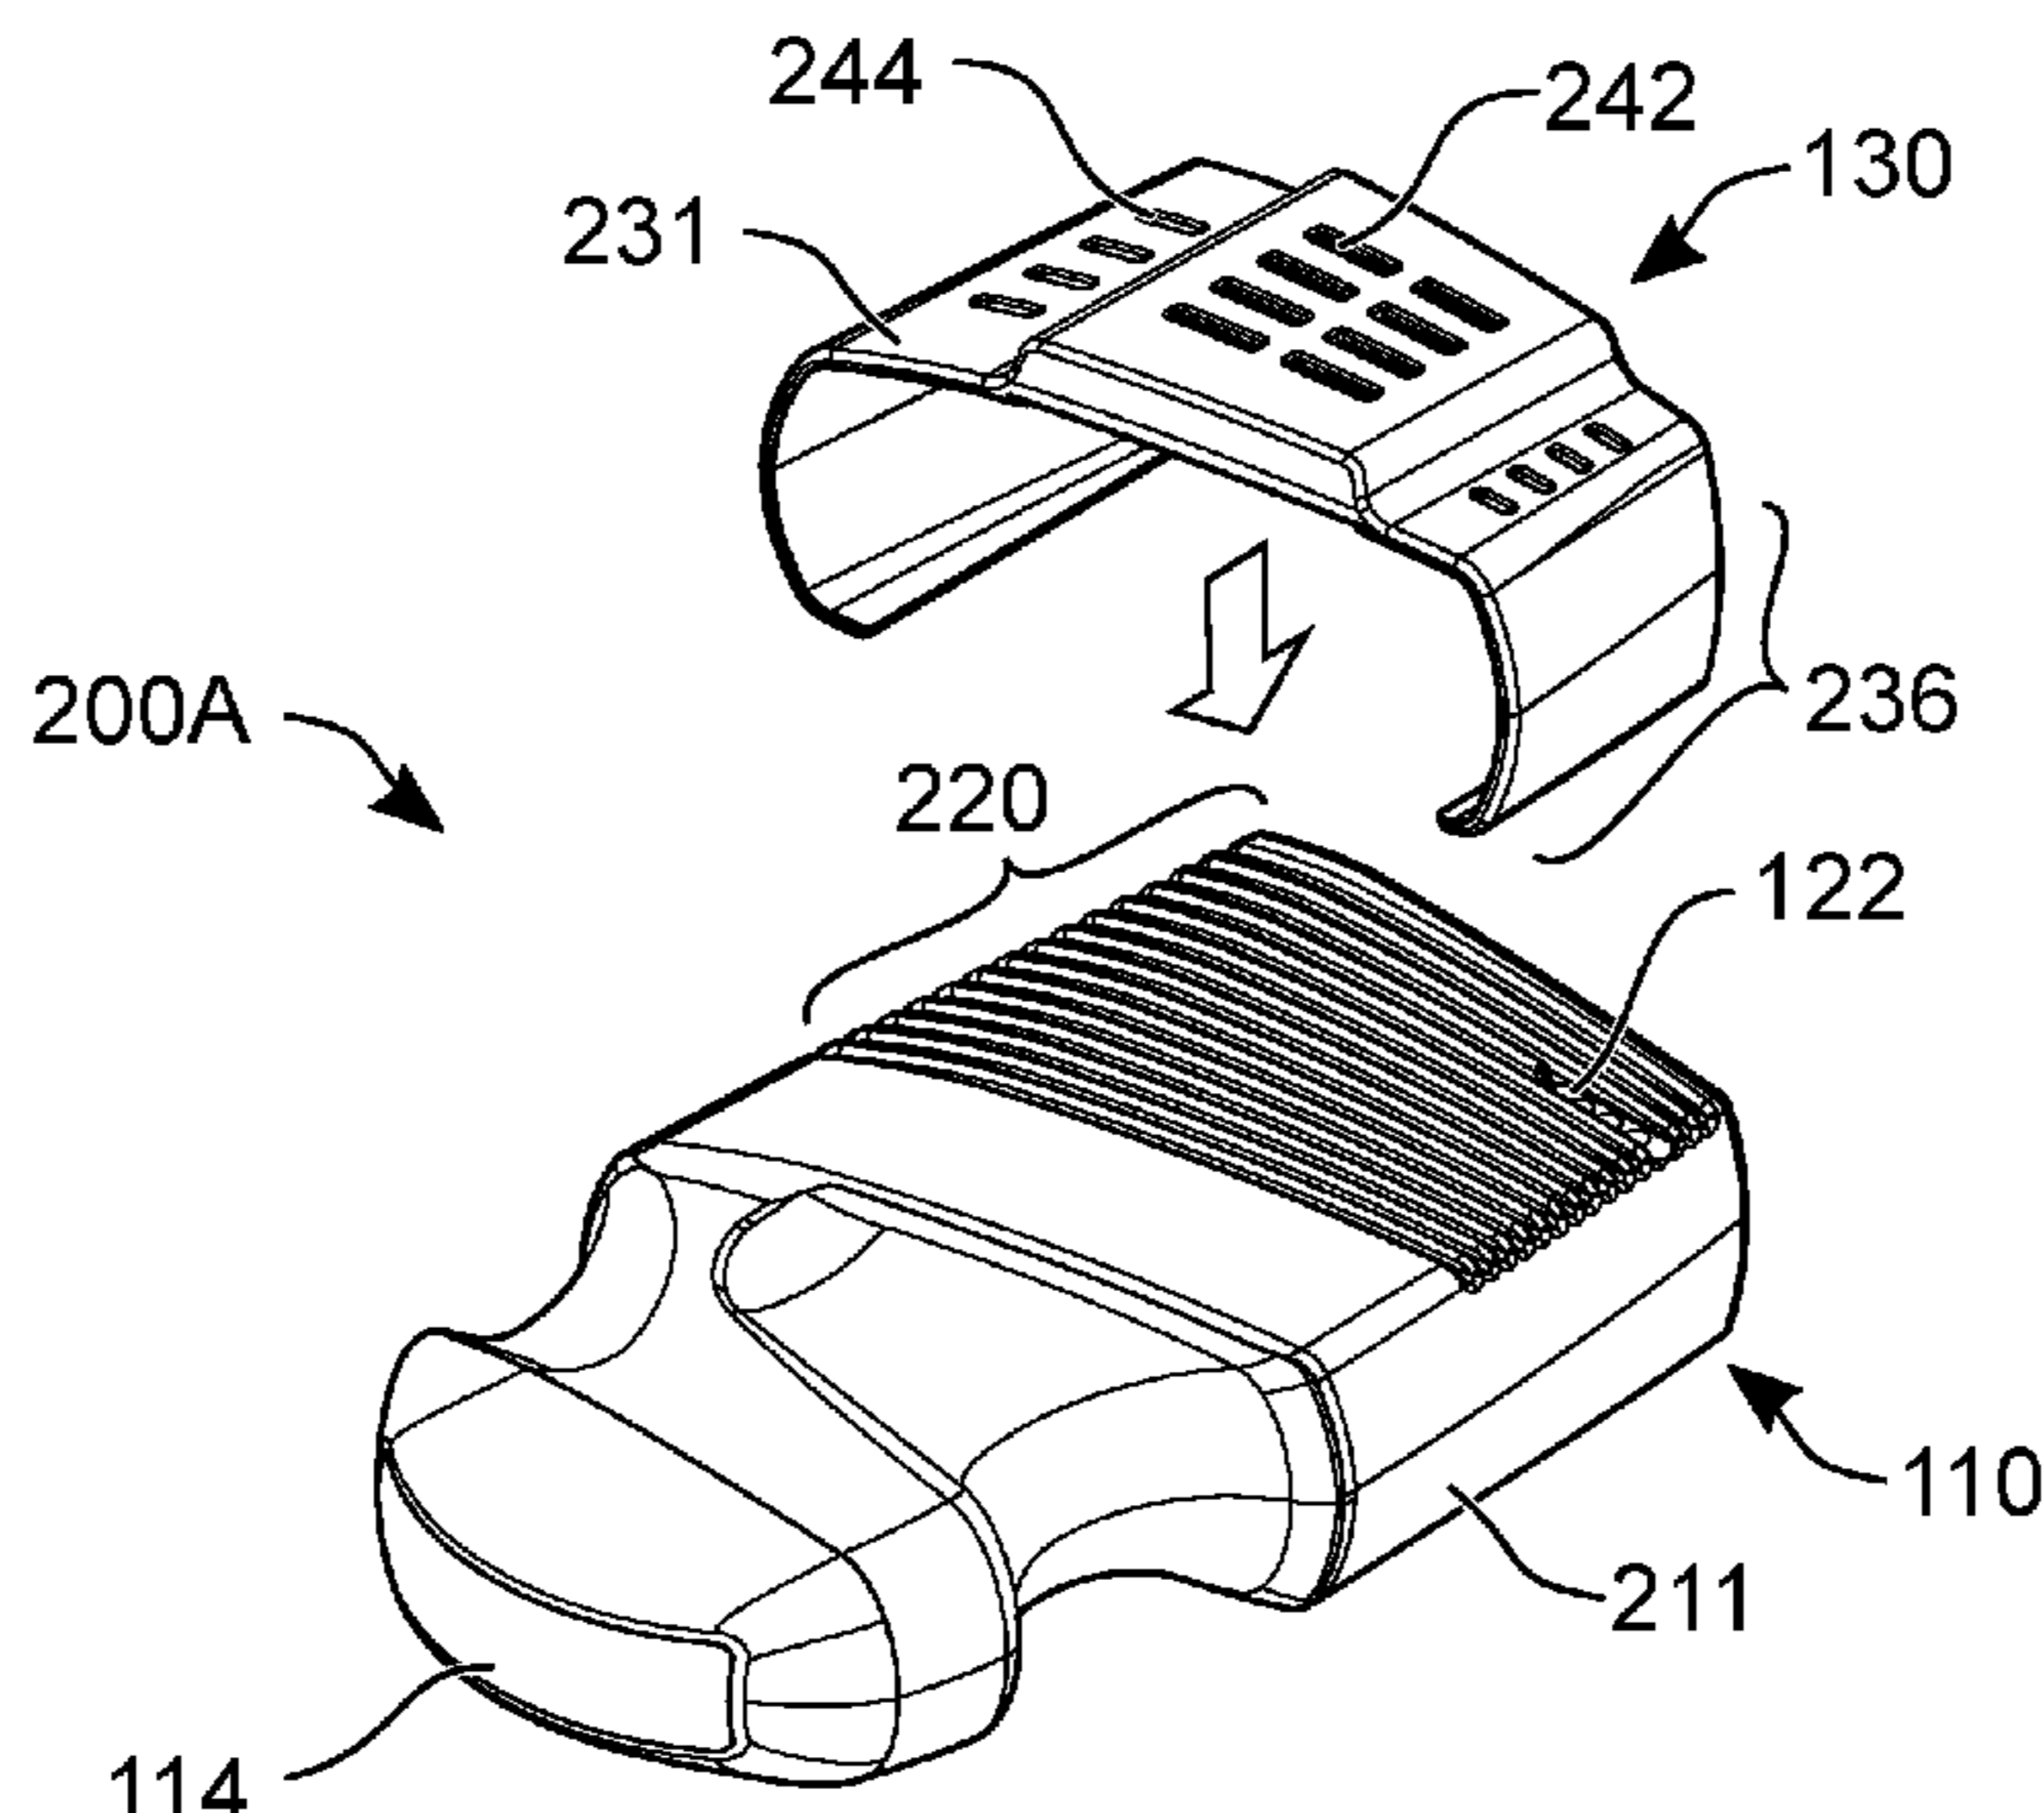

(56)

References Cited

U.S. PATENT DOCUMENTS

8,409,101	B2	4/2013	Hongou et al.	
8,475,375	B2	7/2013	Smith et al.	
2004/0002655	A1	1/2004	Bolorforosh et al.	
2004/0073113	A1	4/2004	Salgo et al.	
2004/0179332	A1*	9/2004	Smith	G01S 7/52082 361/679.41
2005/0075573	A1	4/2005	Park et al.	
2005/0148878	A1	7/2005	Phelps et al.	
2006/0082966	A1	4/2006	Lev et al.	
2006/0191344	A1*	8/2006	Hashimoto	A61B 8/00 73/632
2008/0146924	A1	6/2008	Smith et al.	
2009/0261804	A1*	10/2009	McKenna	A61B 18/1442 324/71.1
2010/0331702	A1*	12/2010	Hongou	A61B 8/14 600/459
2011/0096497	A1	4/2011	Huang	
2016/0077059	A1	3/2016	Chung et al.	
2016/0242747	A1*	8/2016	Siedenburg	A61B 8/546
2017/0020490	A1	1/2017	Ryu et al.	
2017/0043189	A1*	2/2017	Stoddard	A61B 8/4281

* cited by examiner

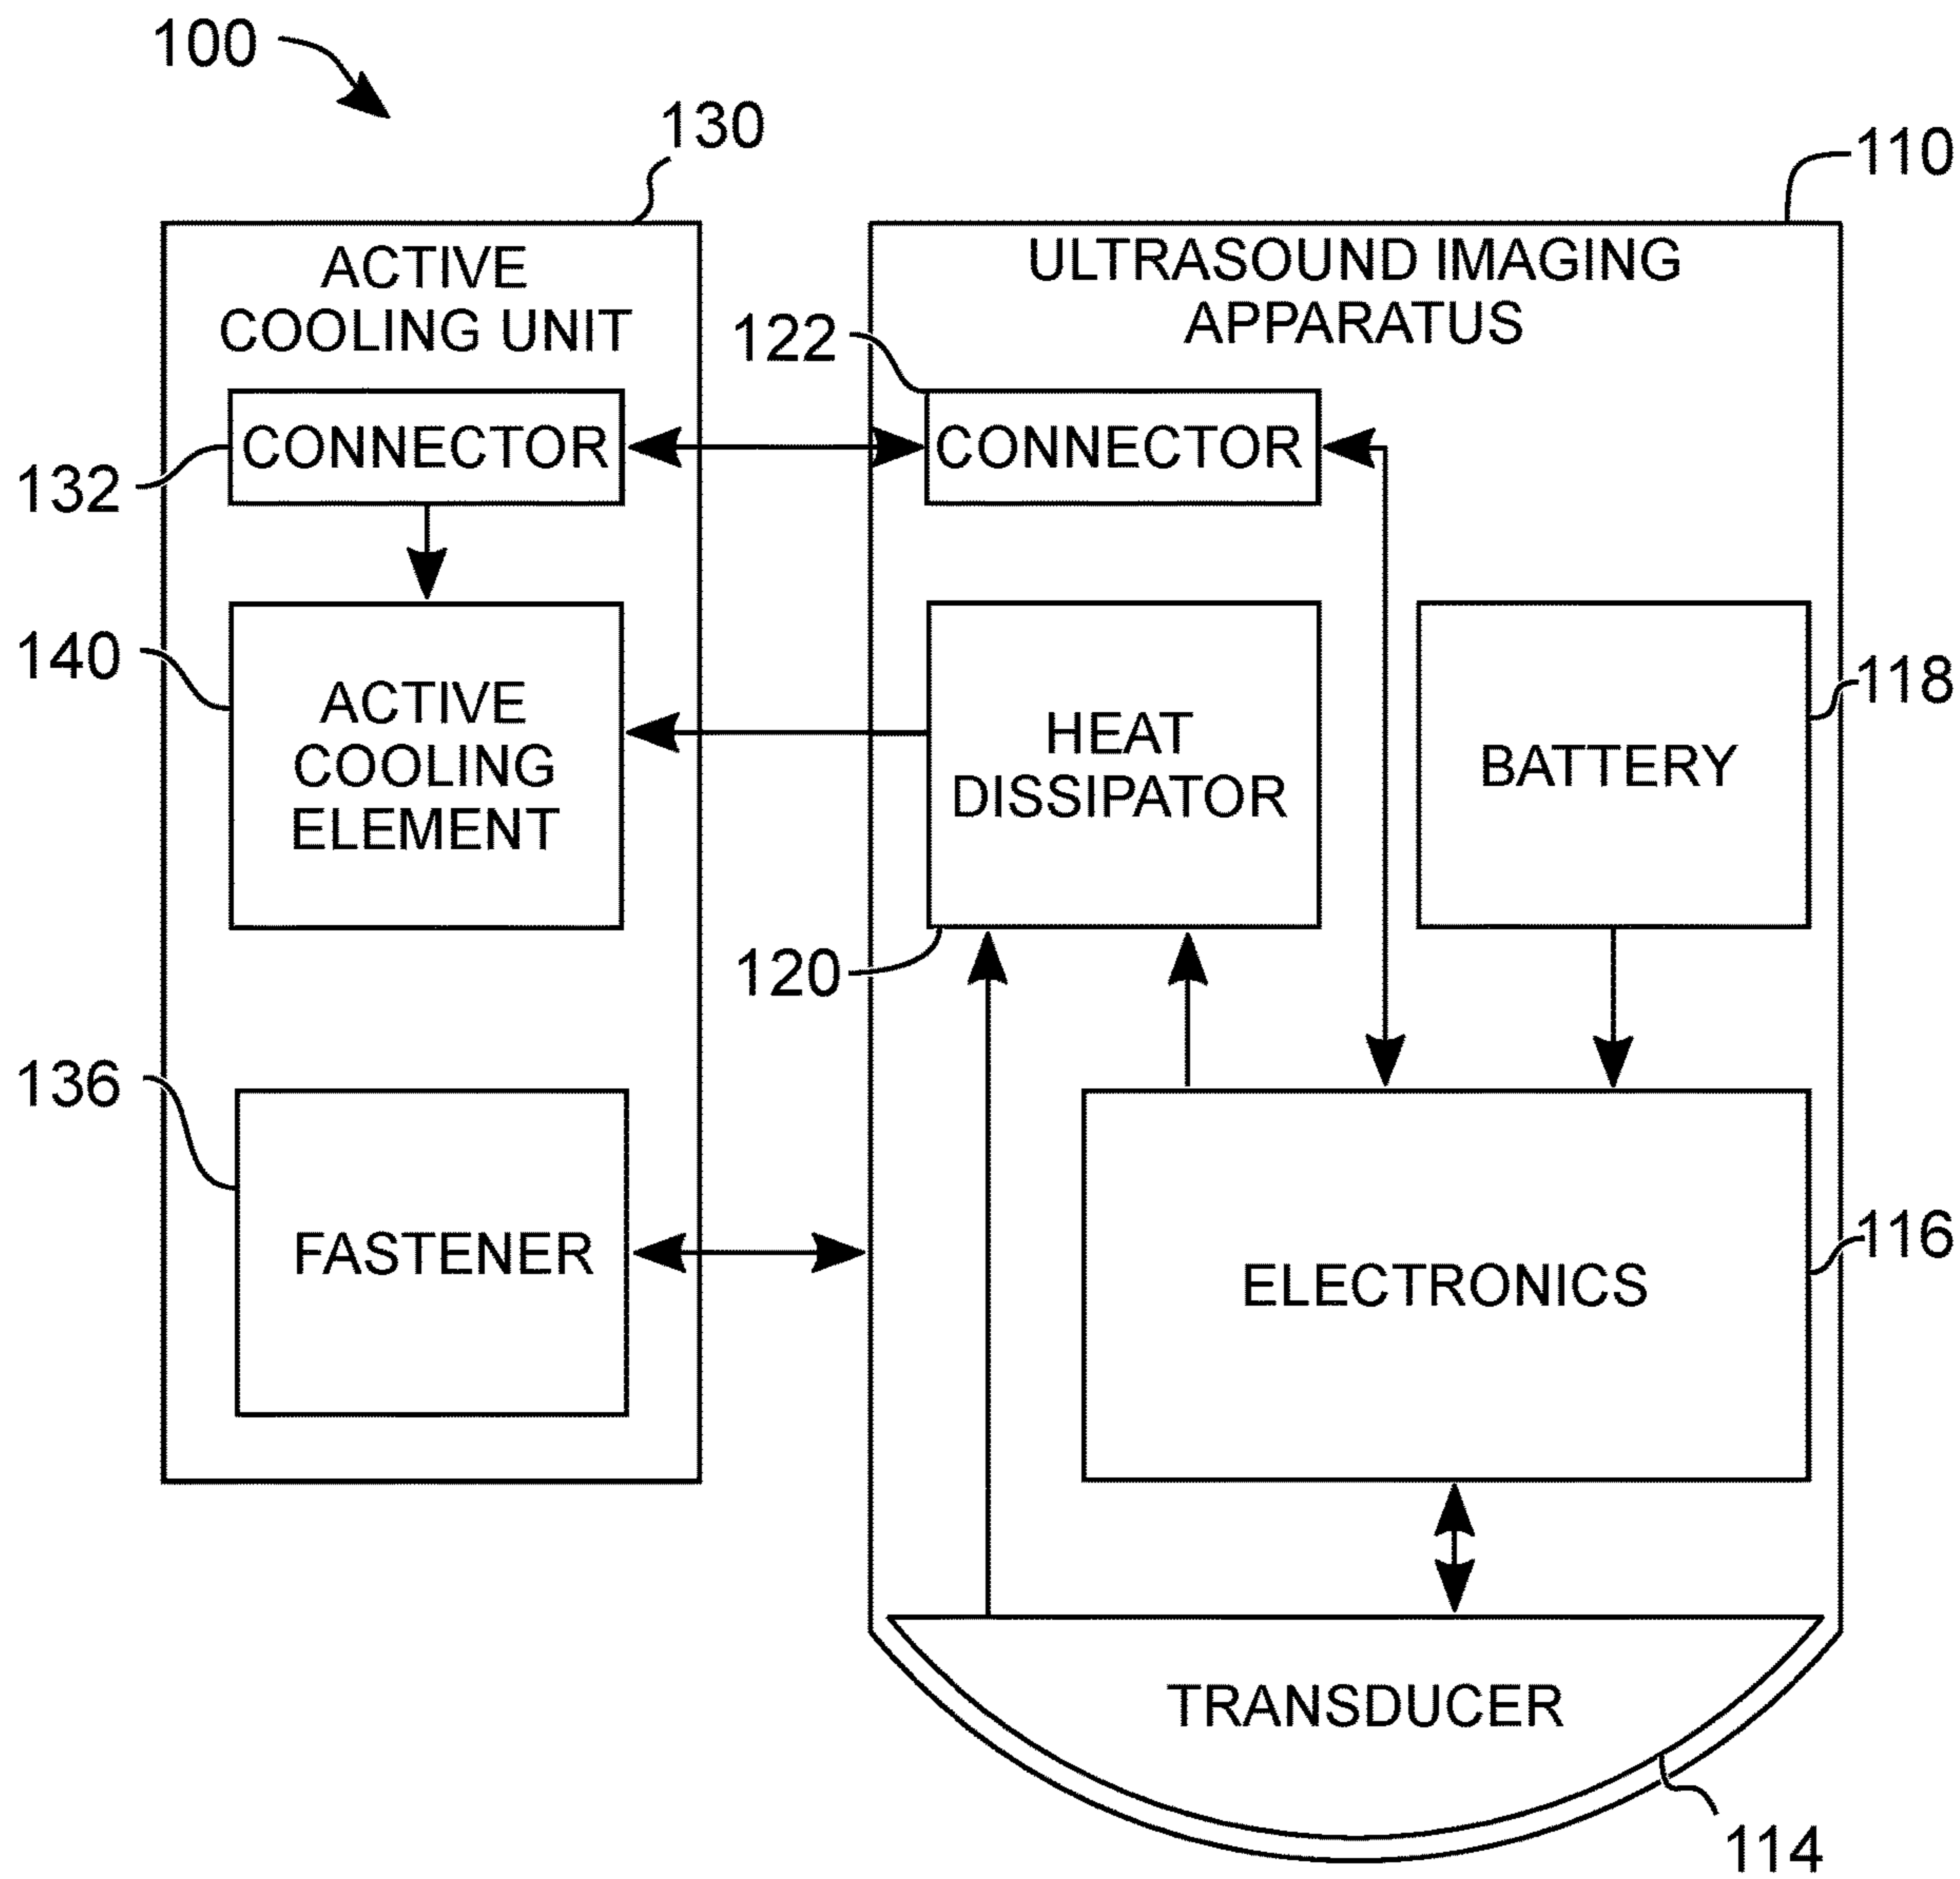


FIG. 1

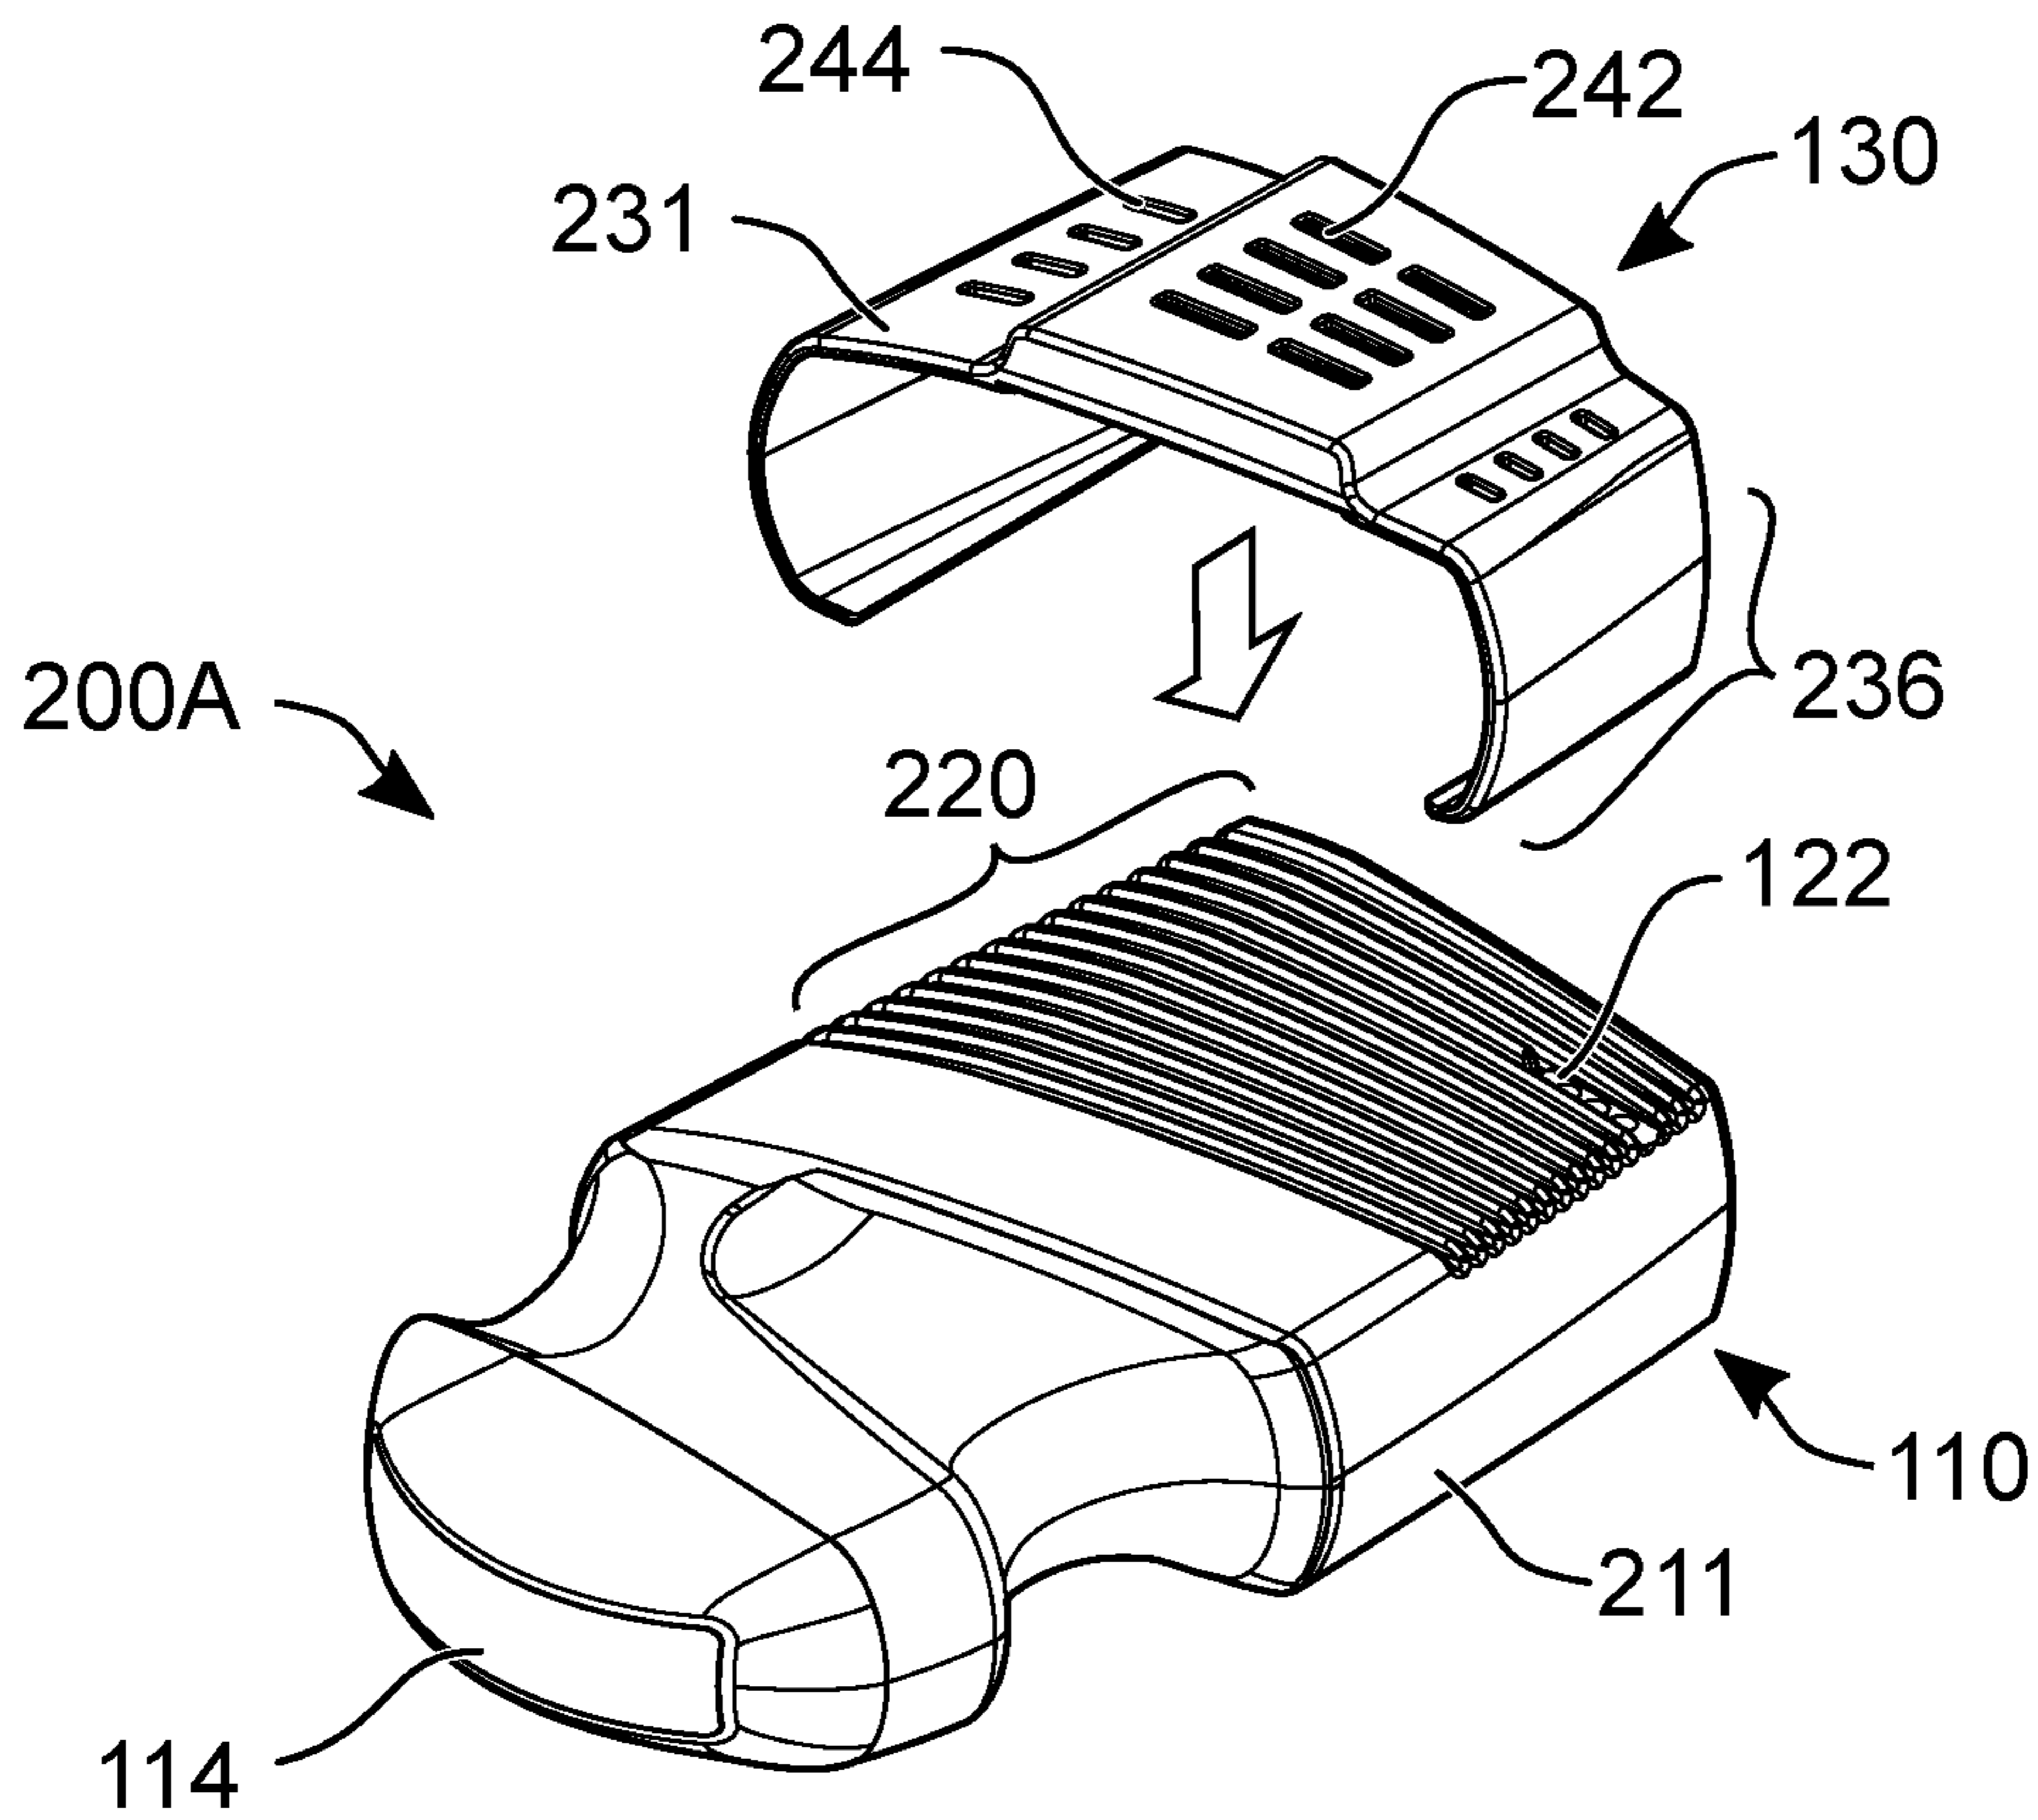


FIG. 2A

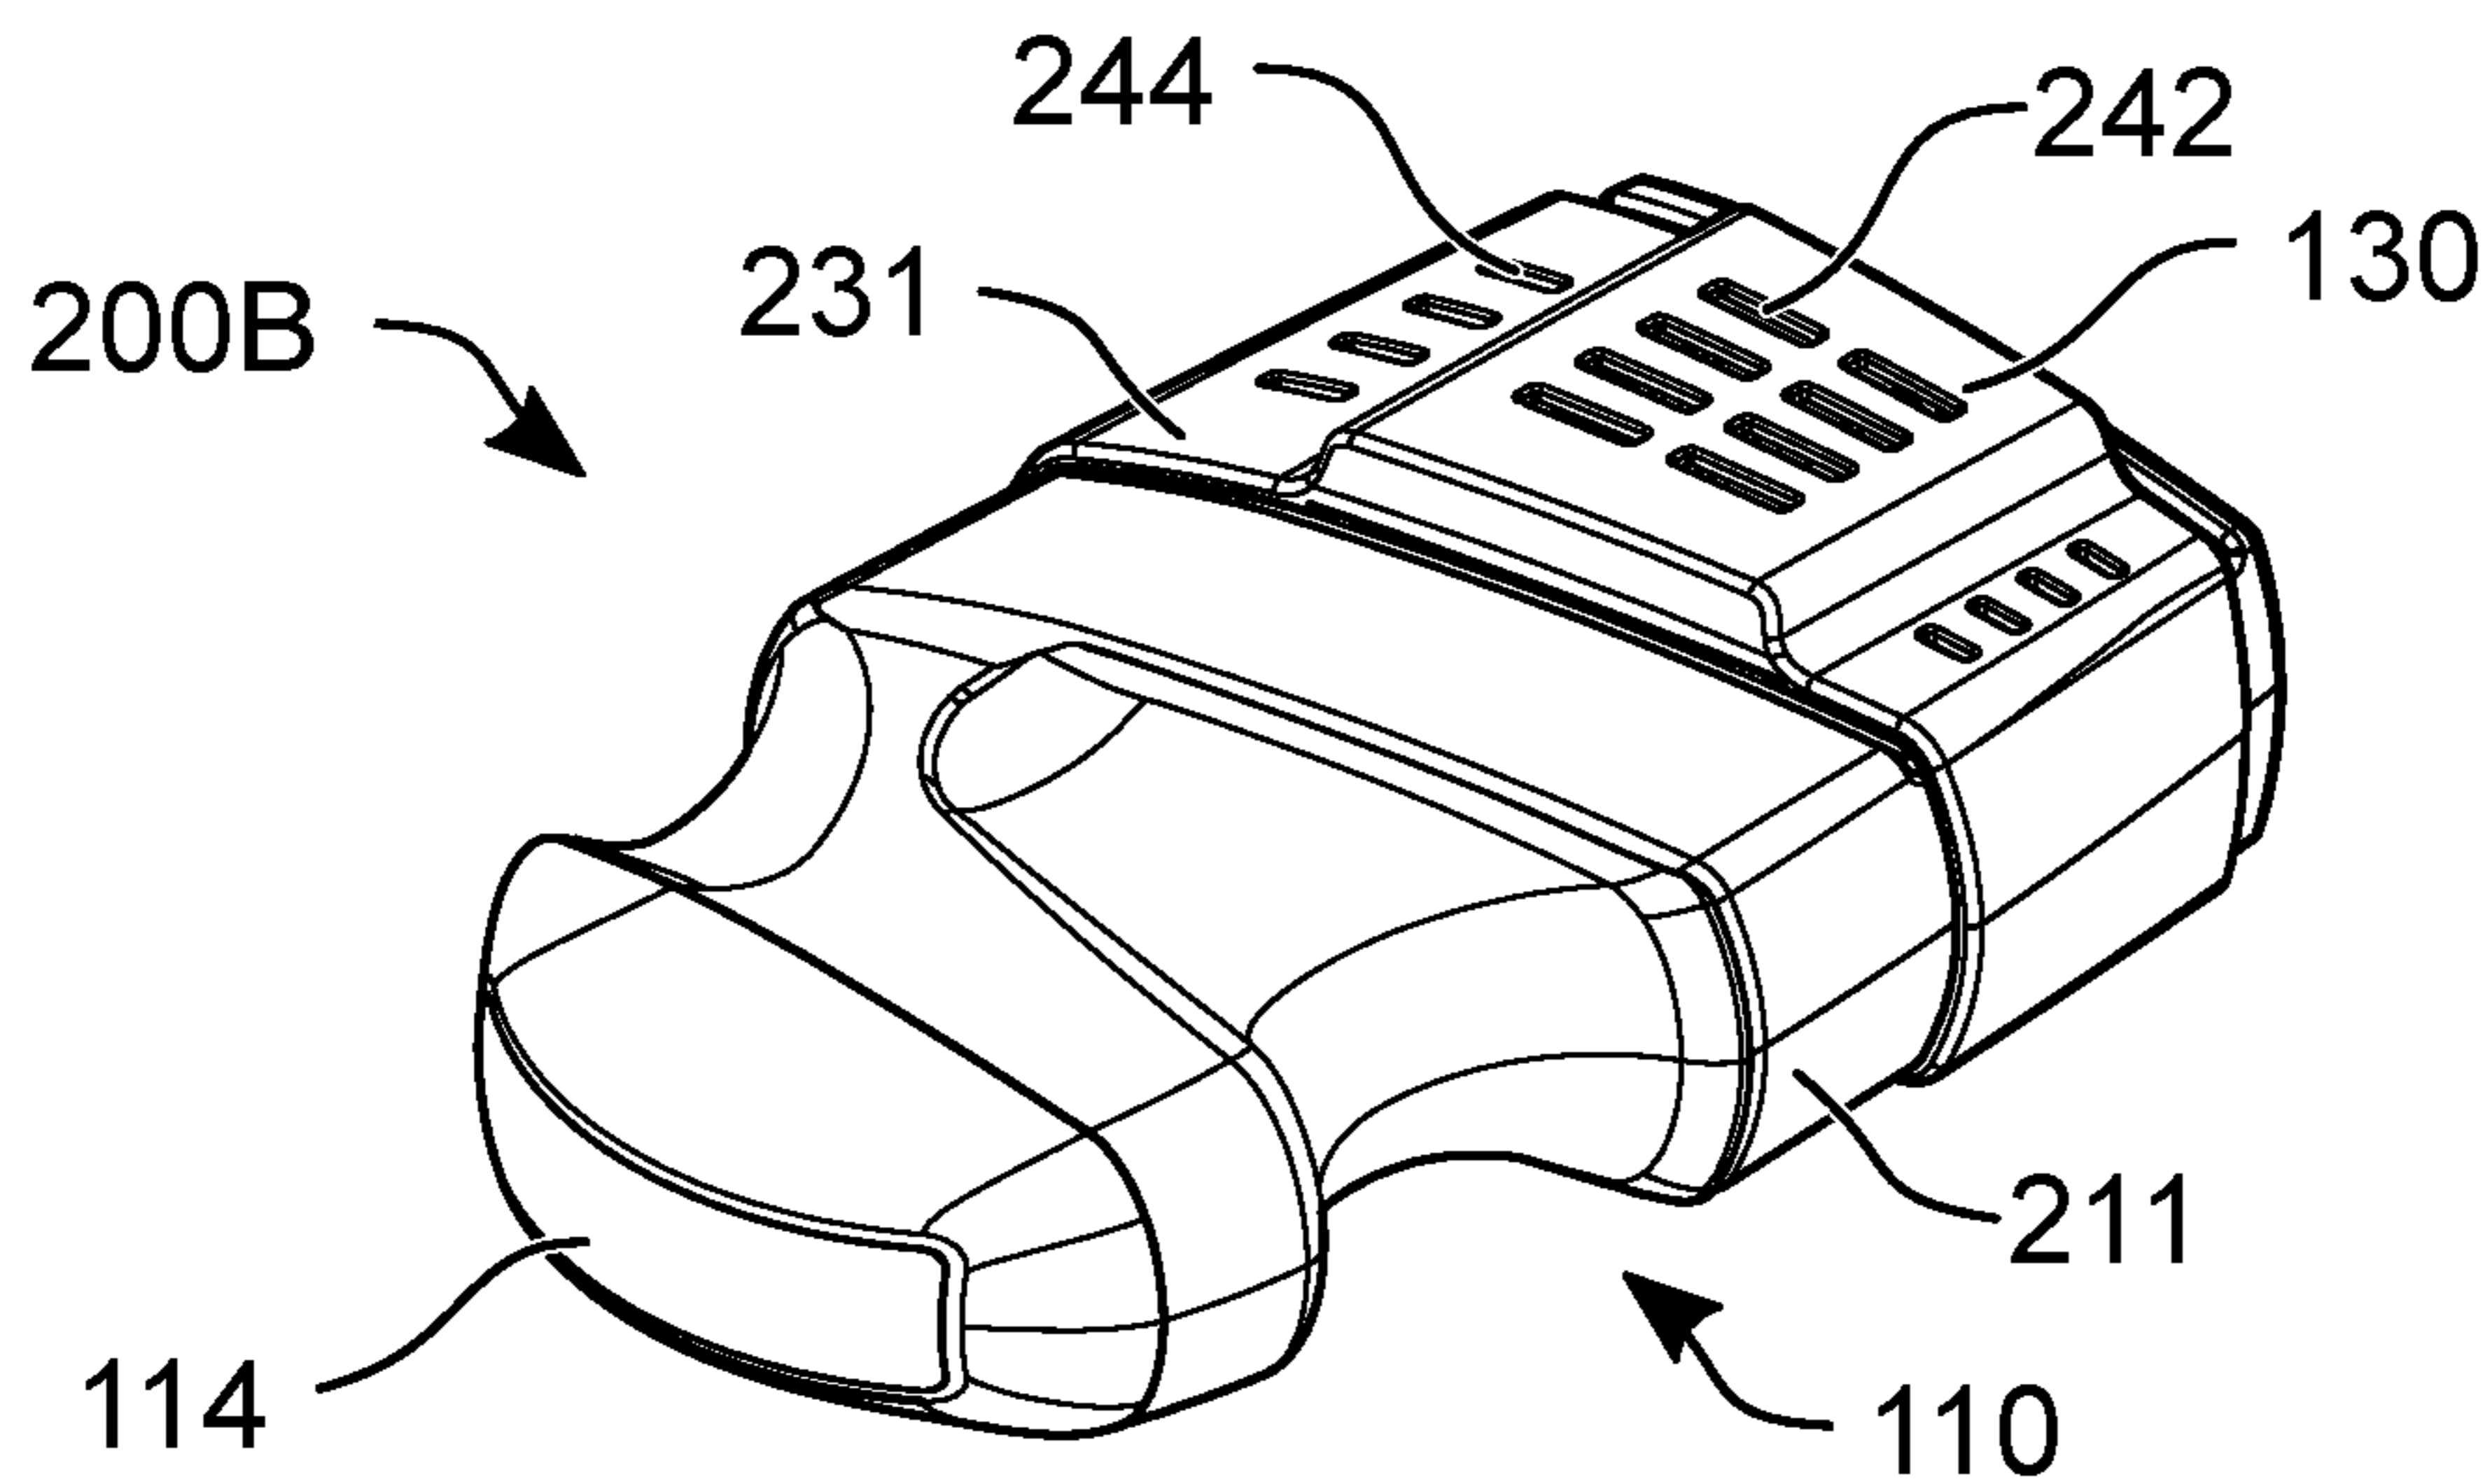


FIG. 2B

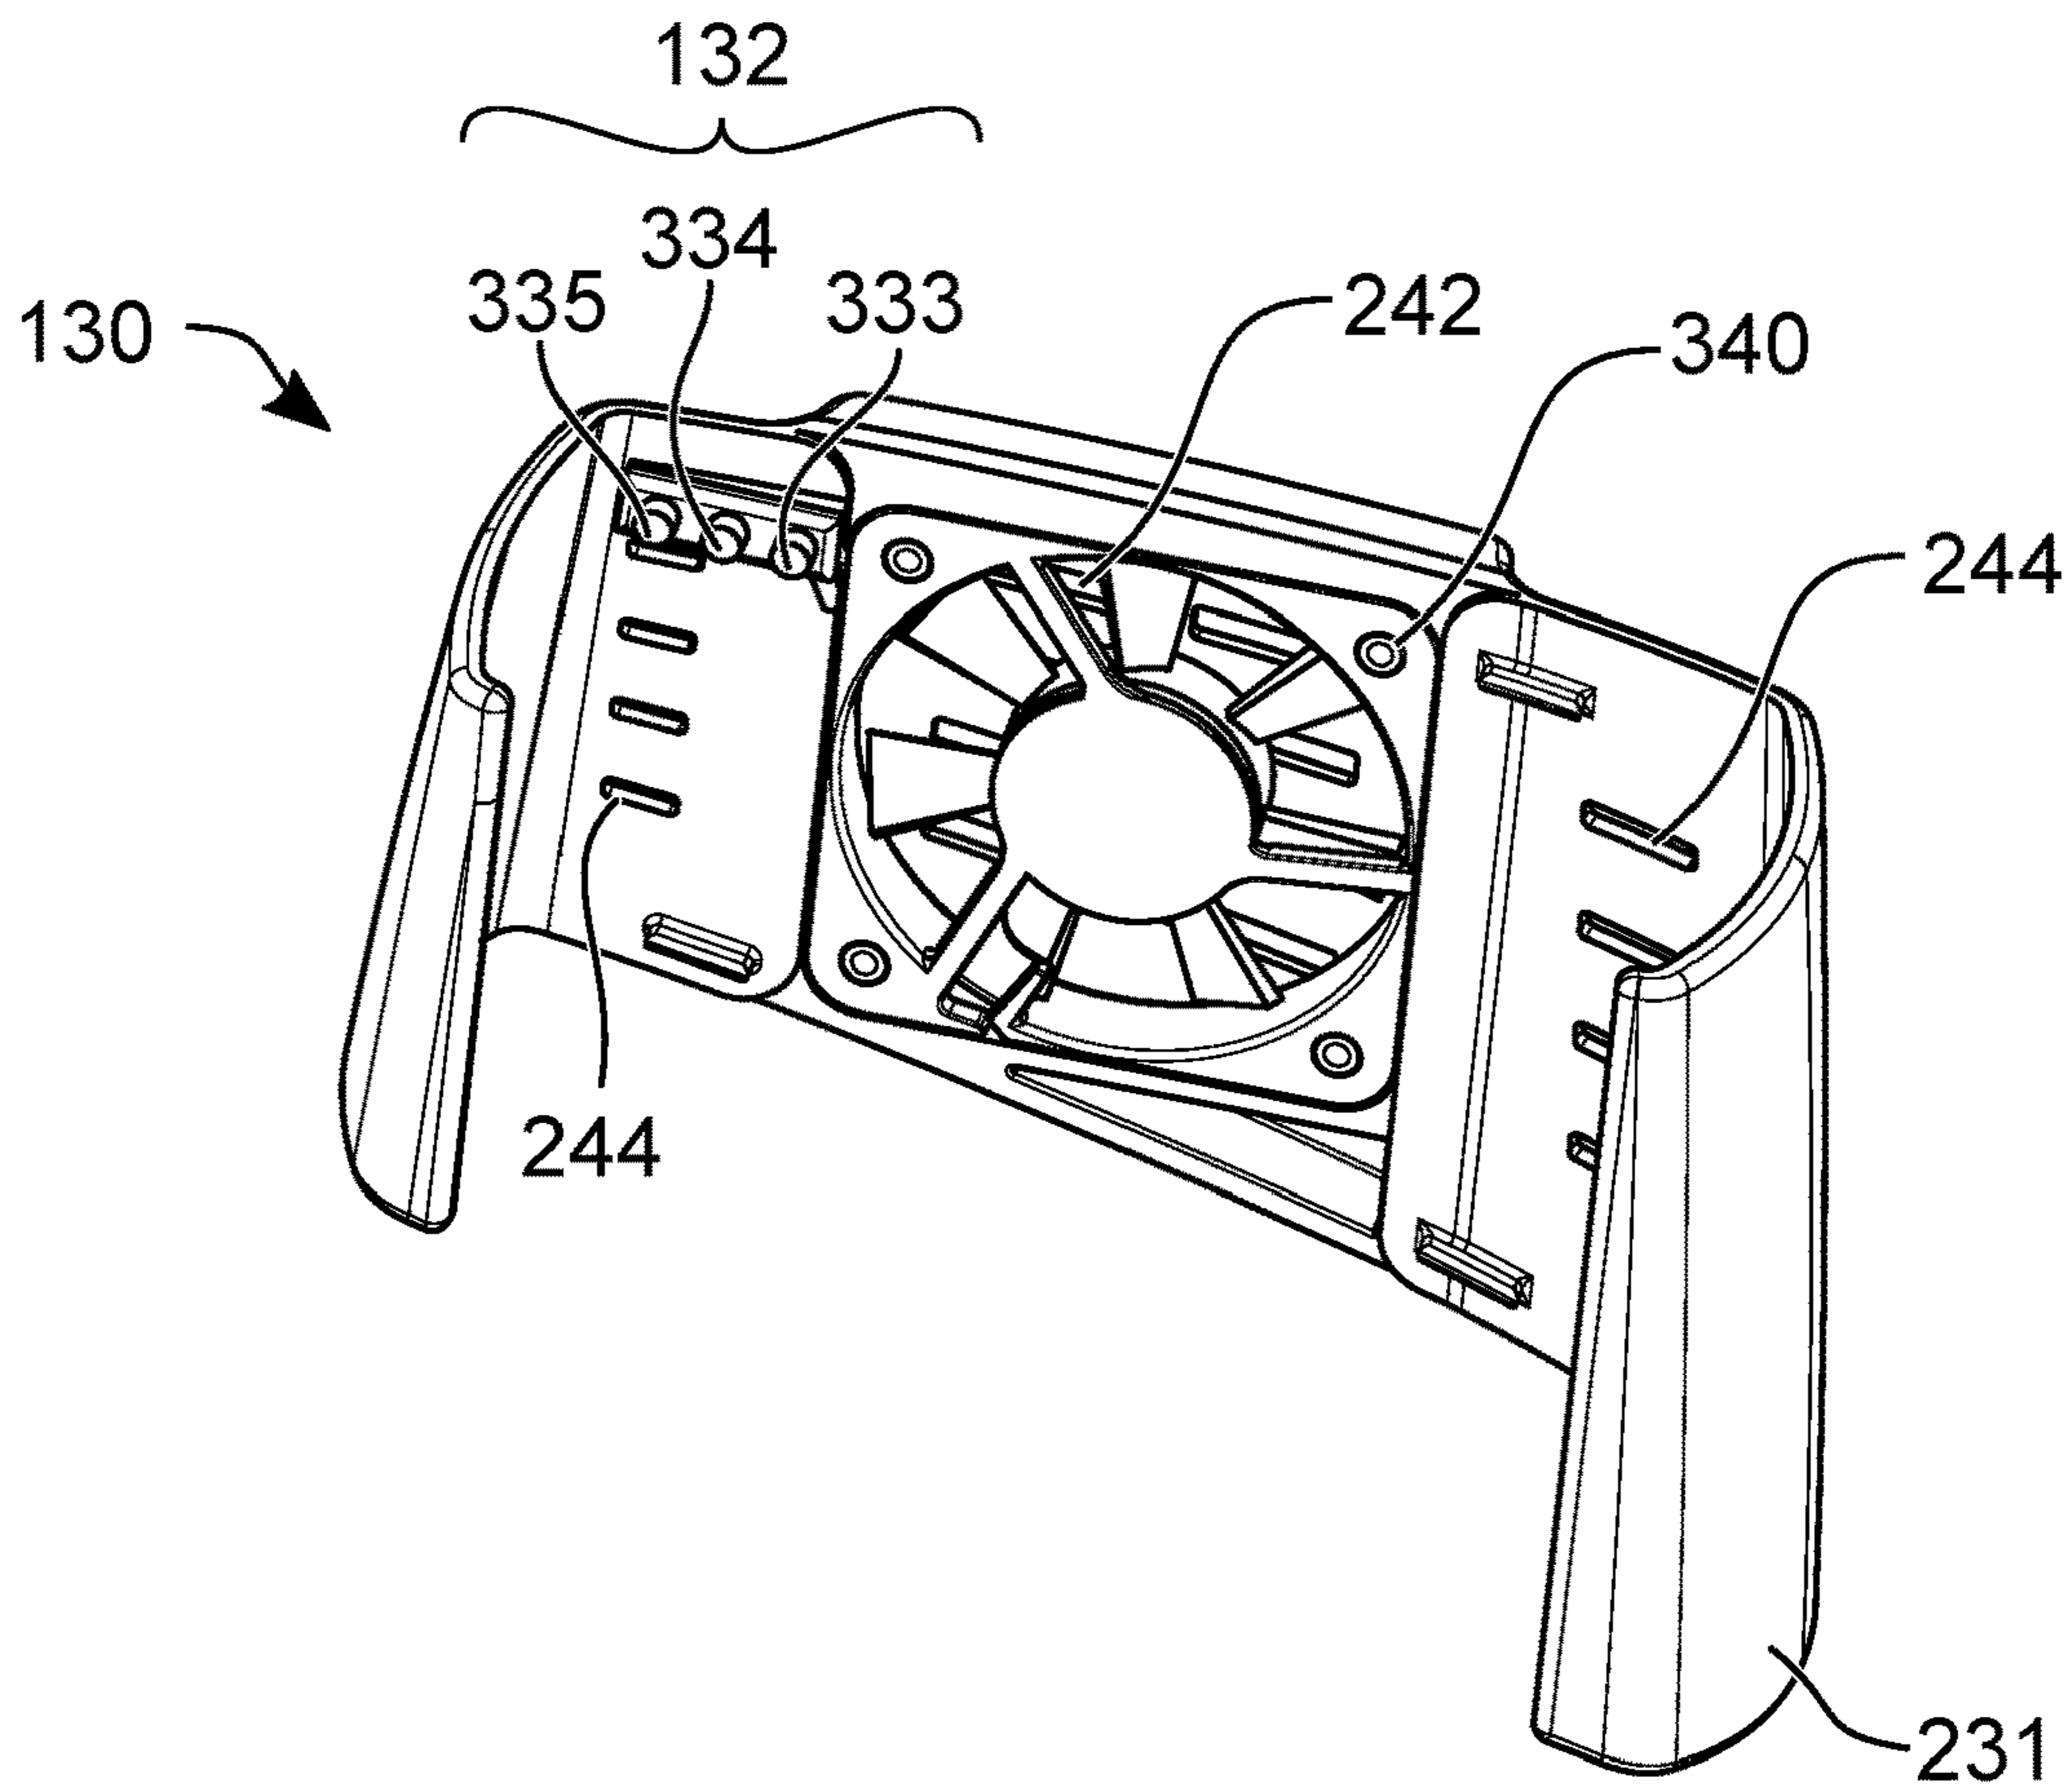


FIG. 3

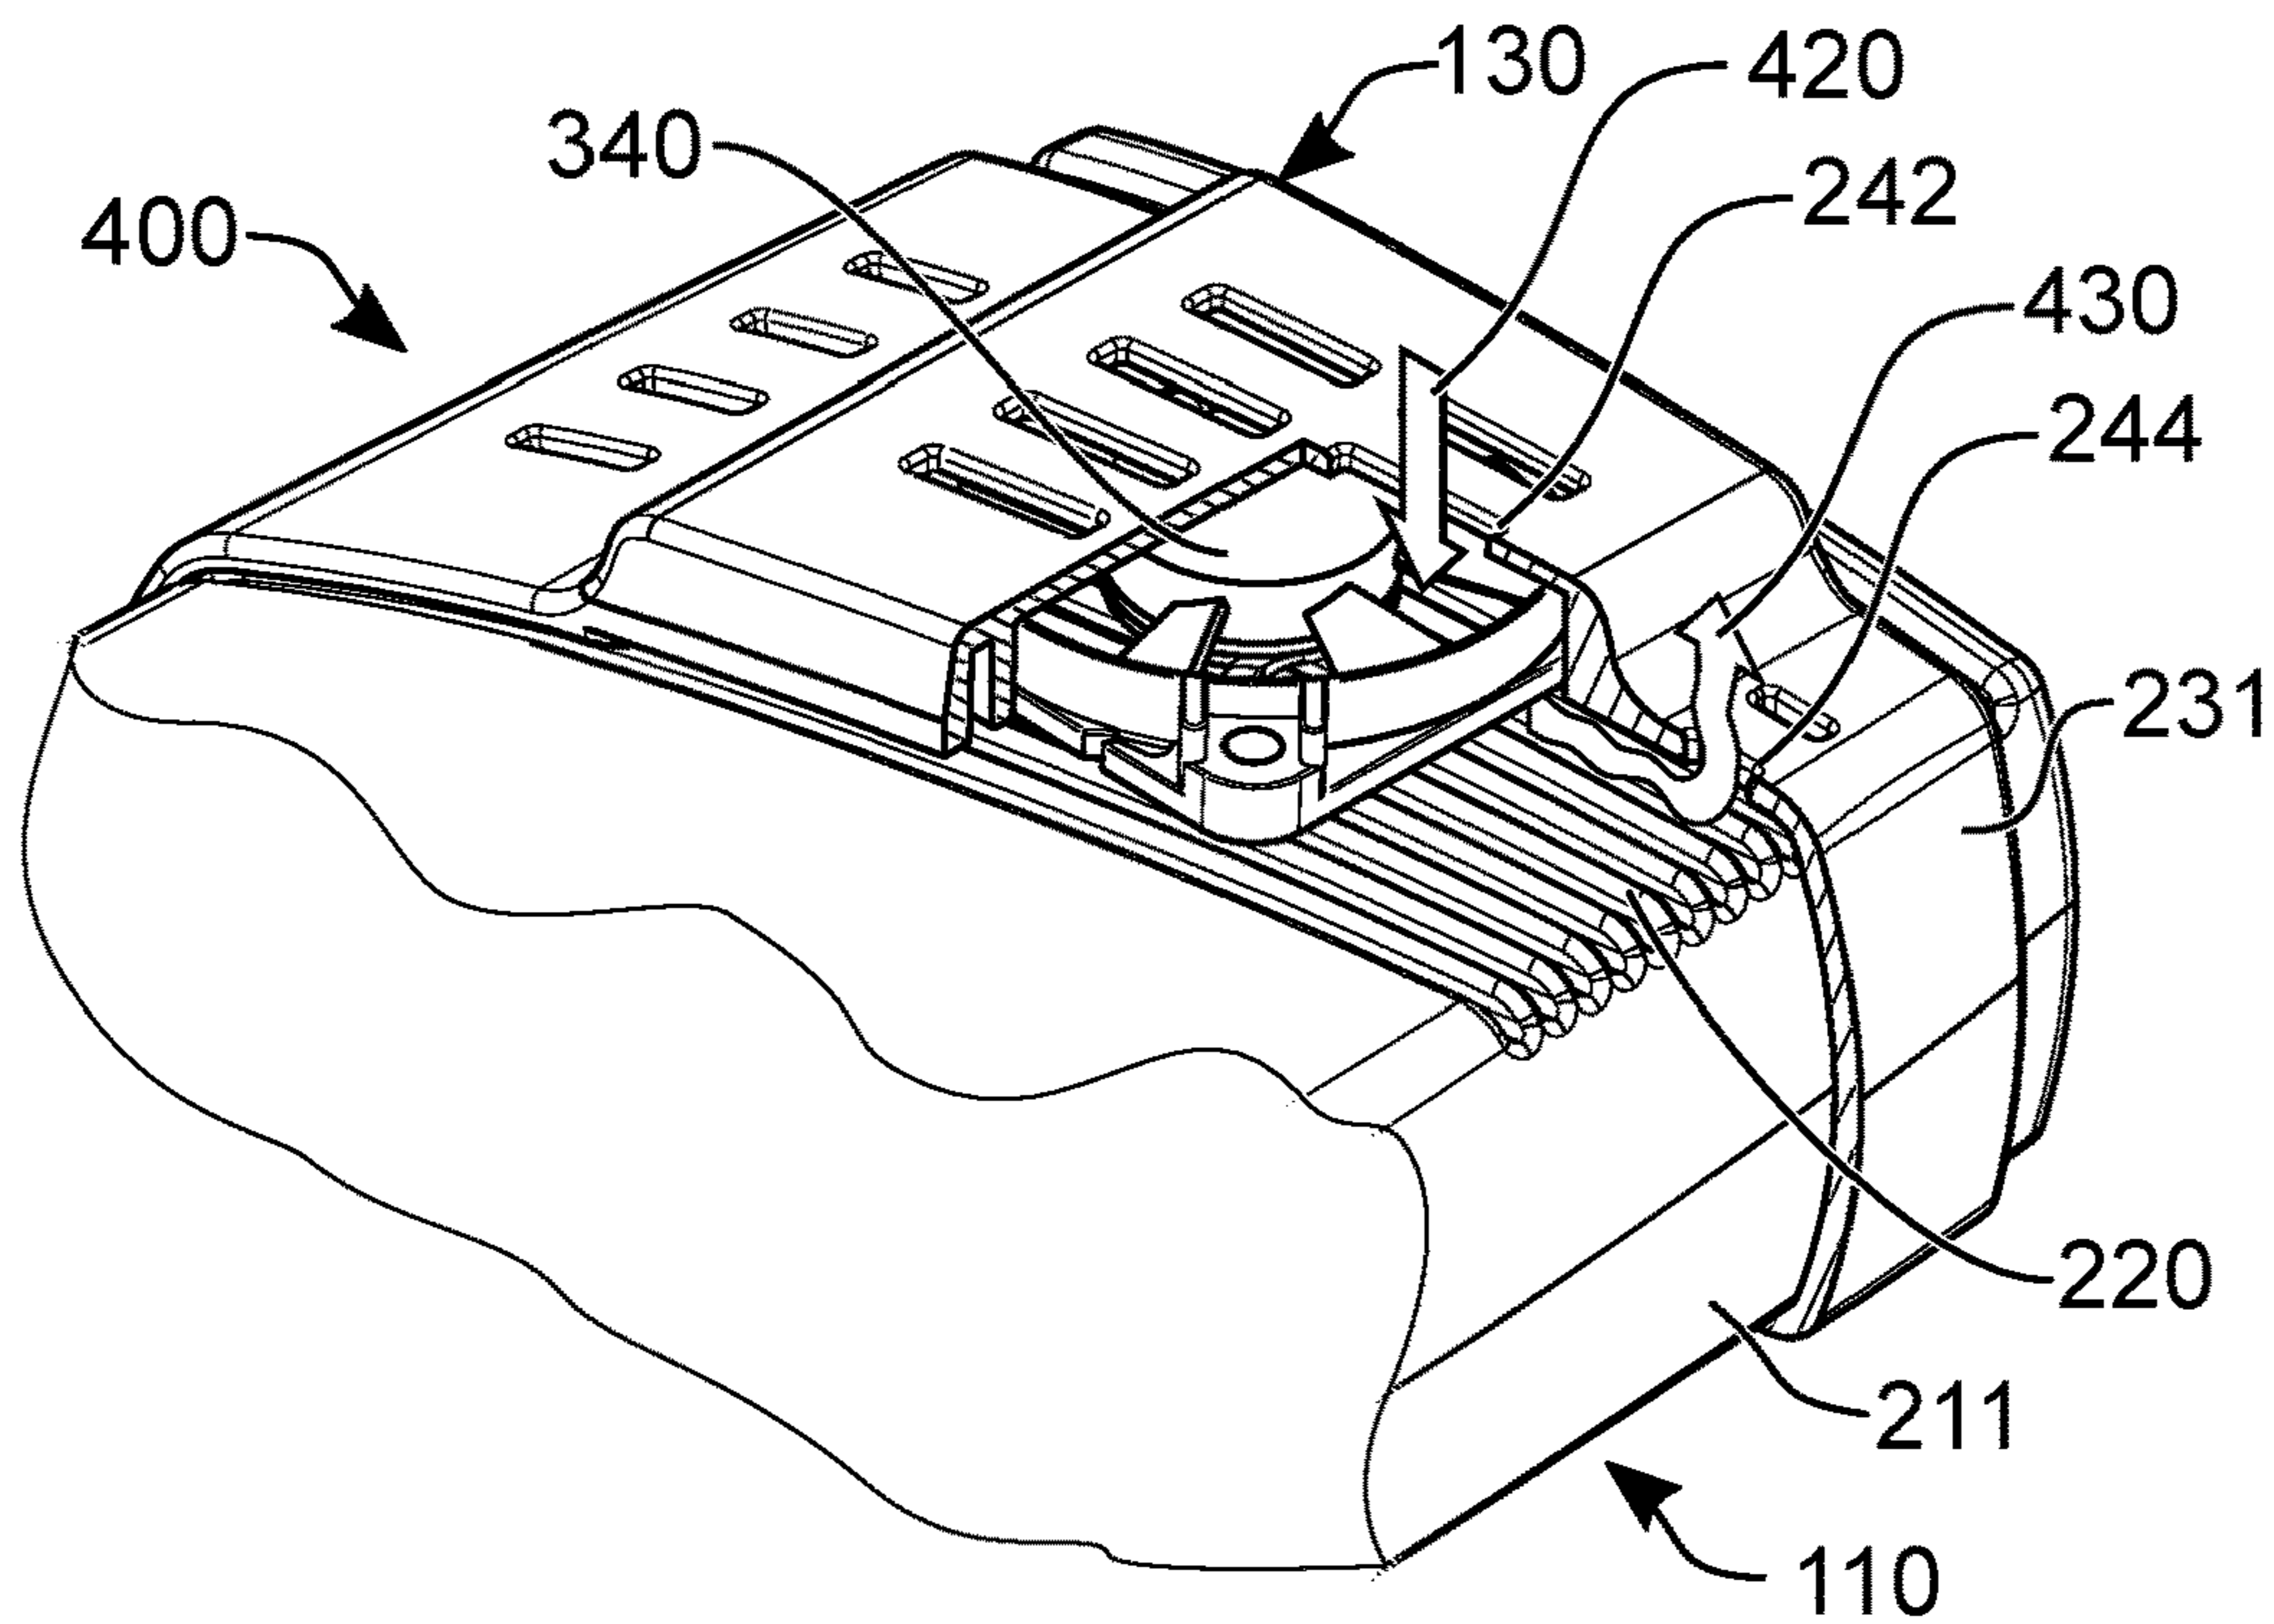


FIG. 4

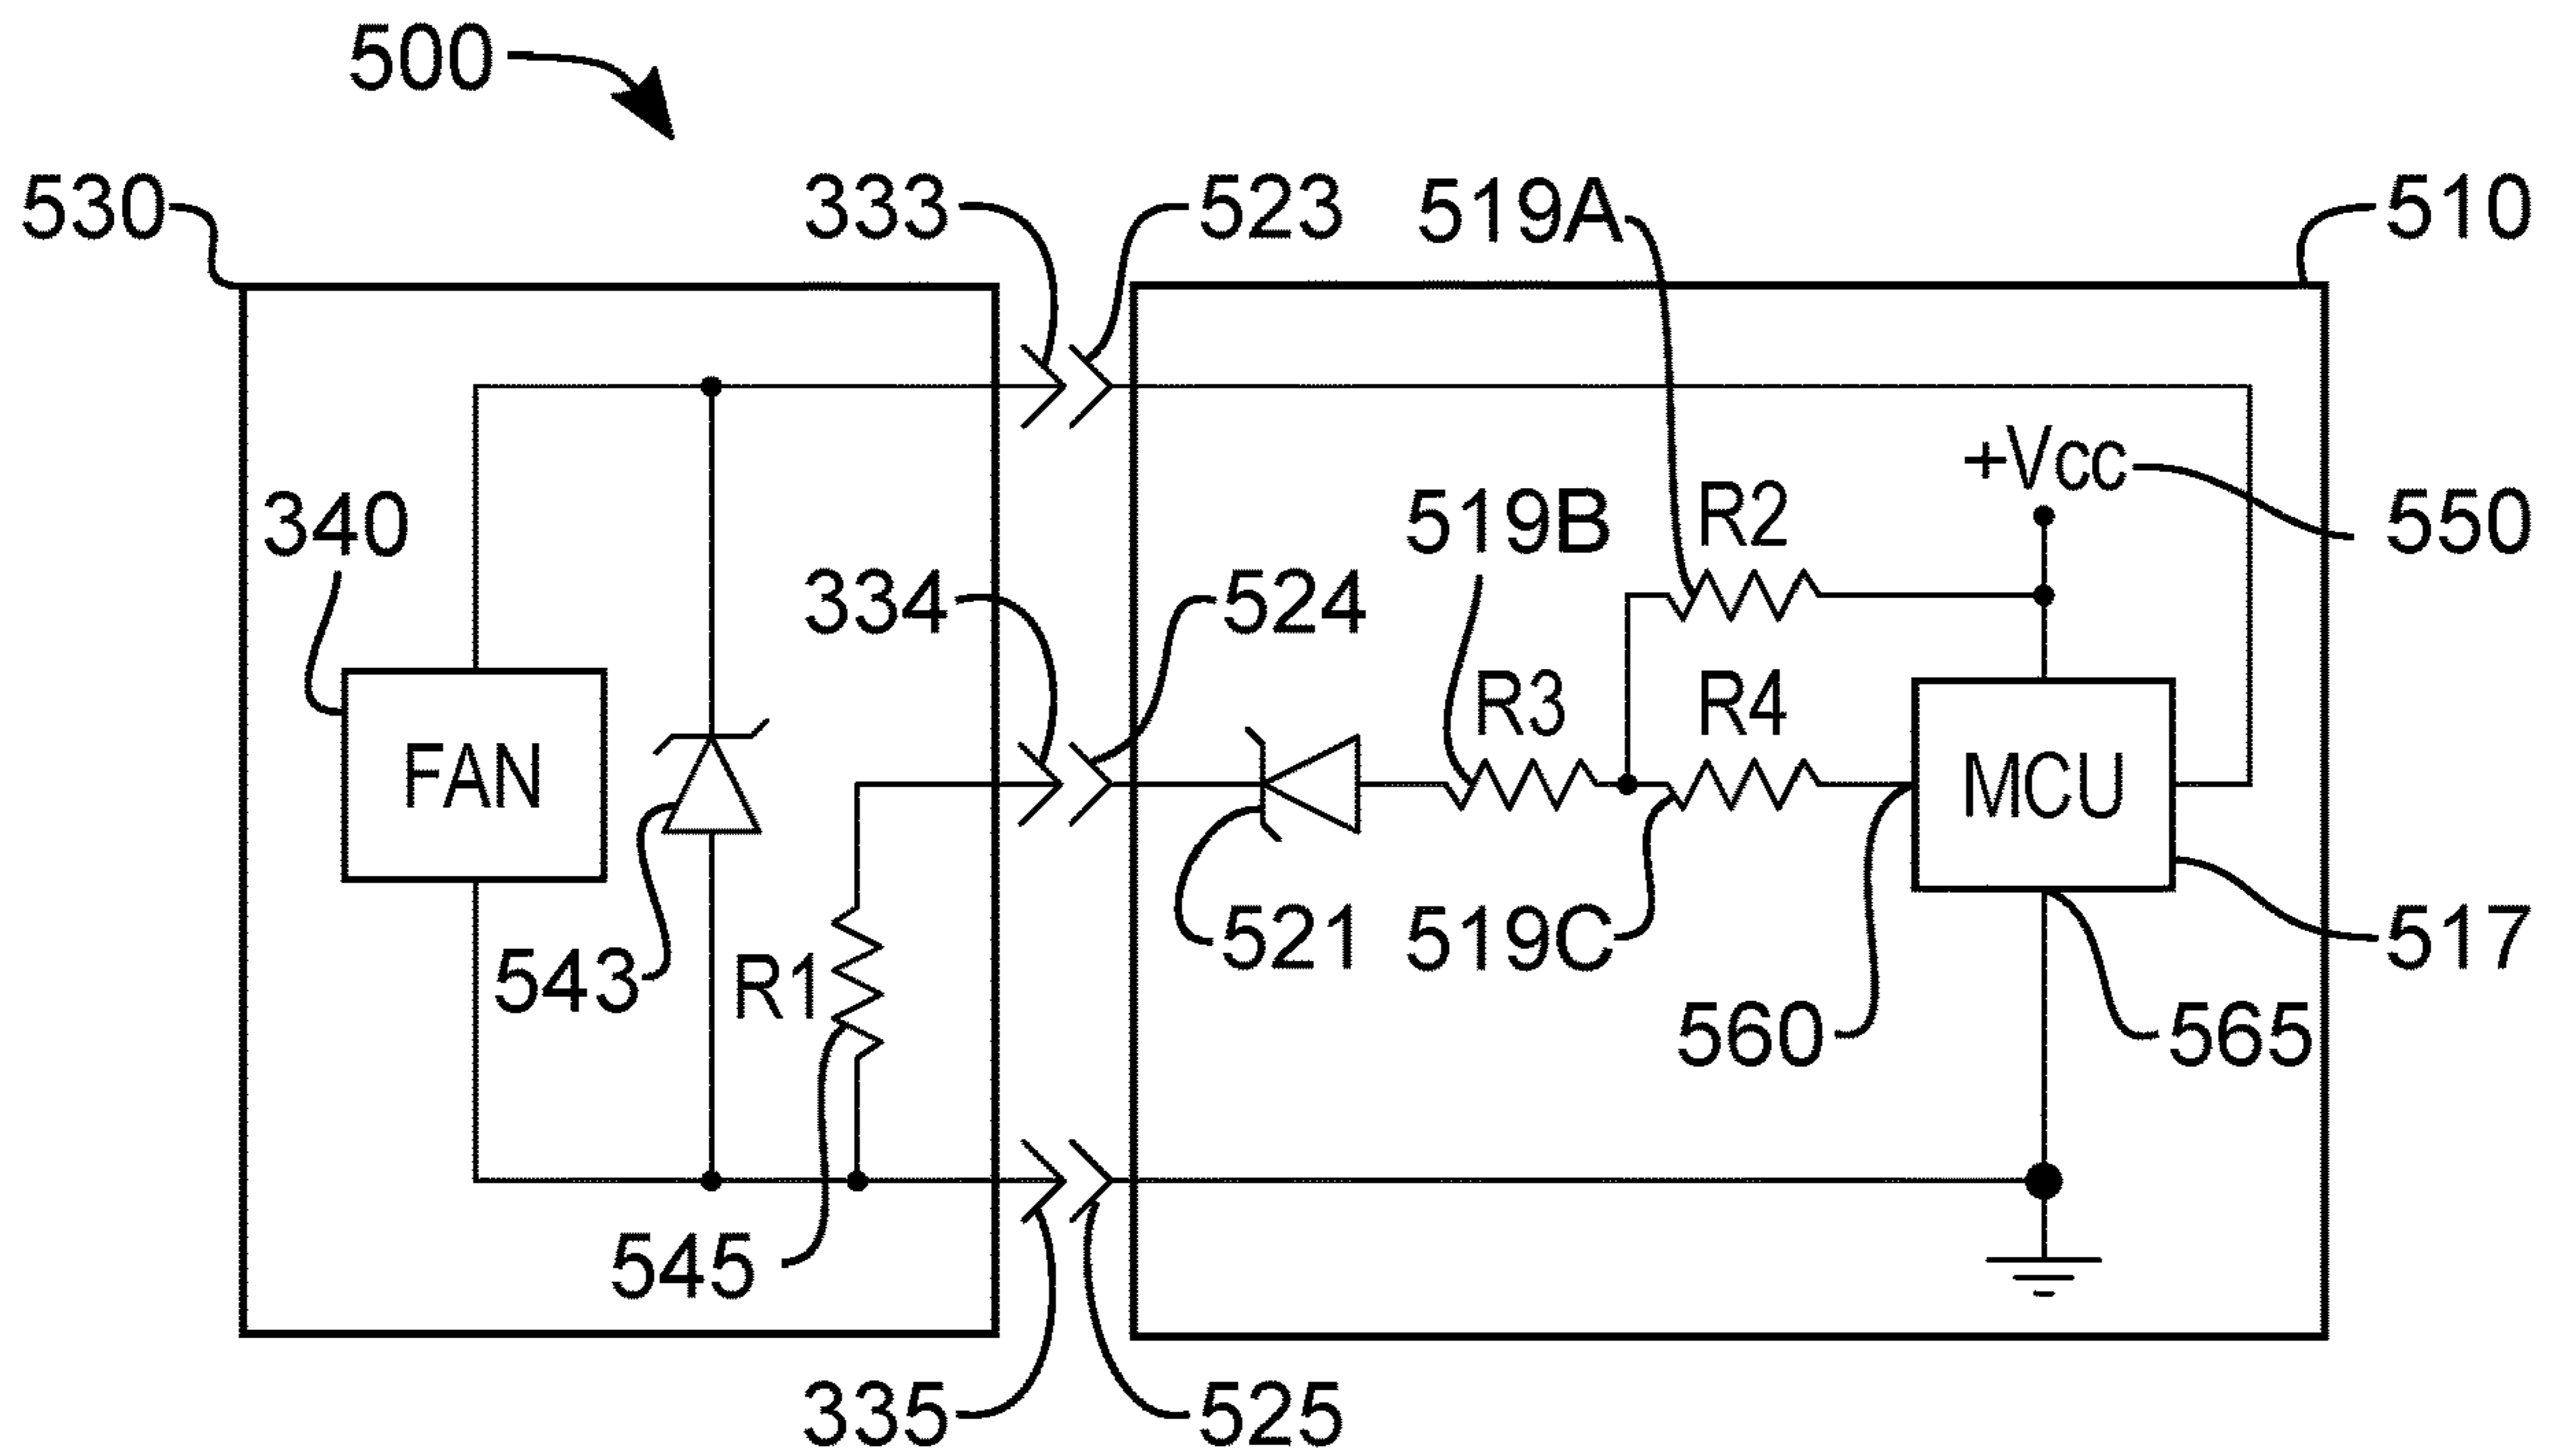


FIG. 5

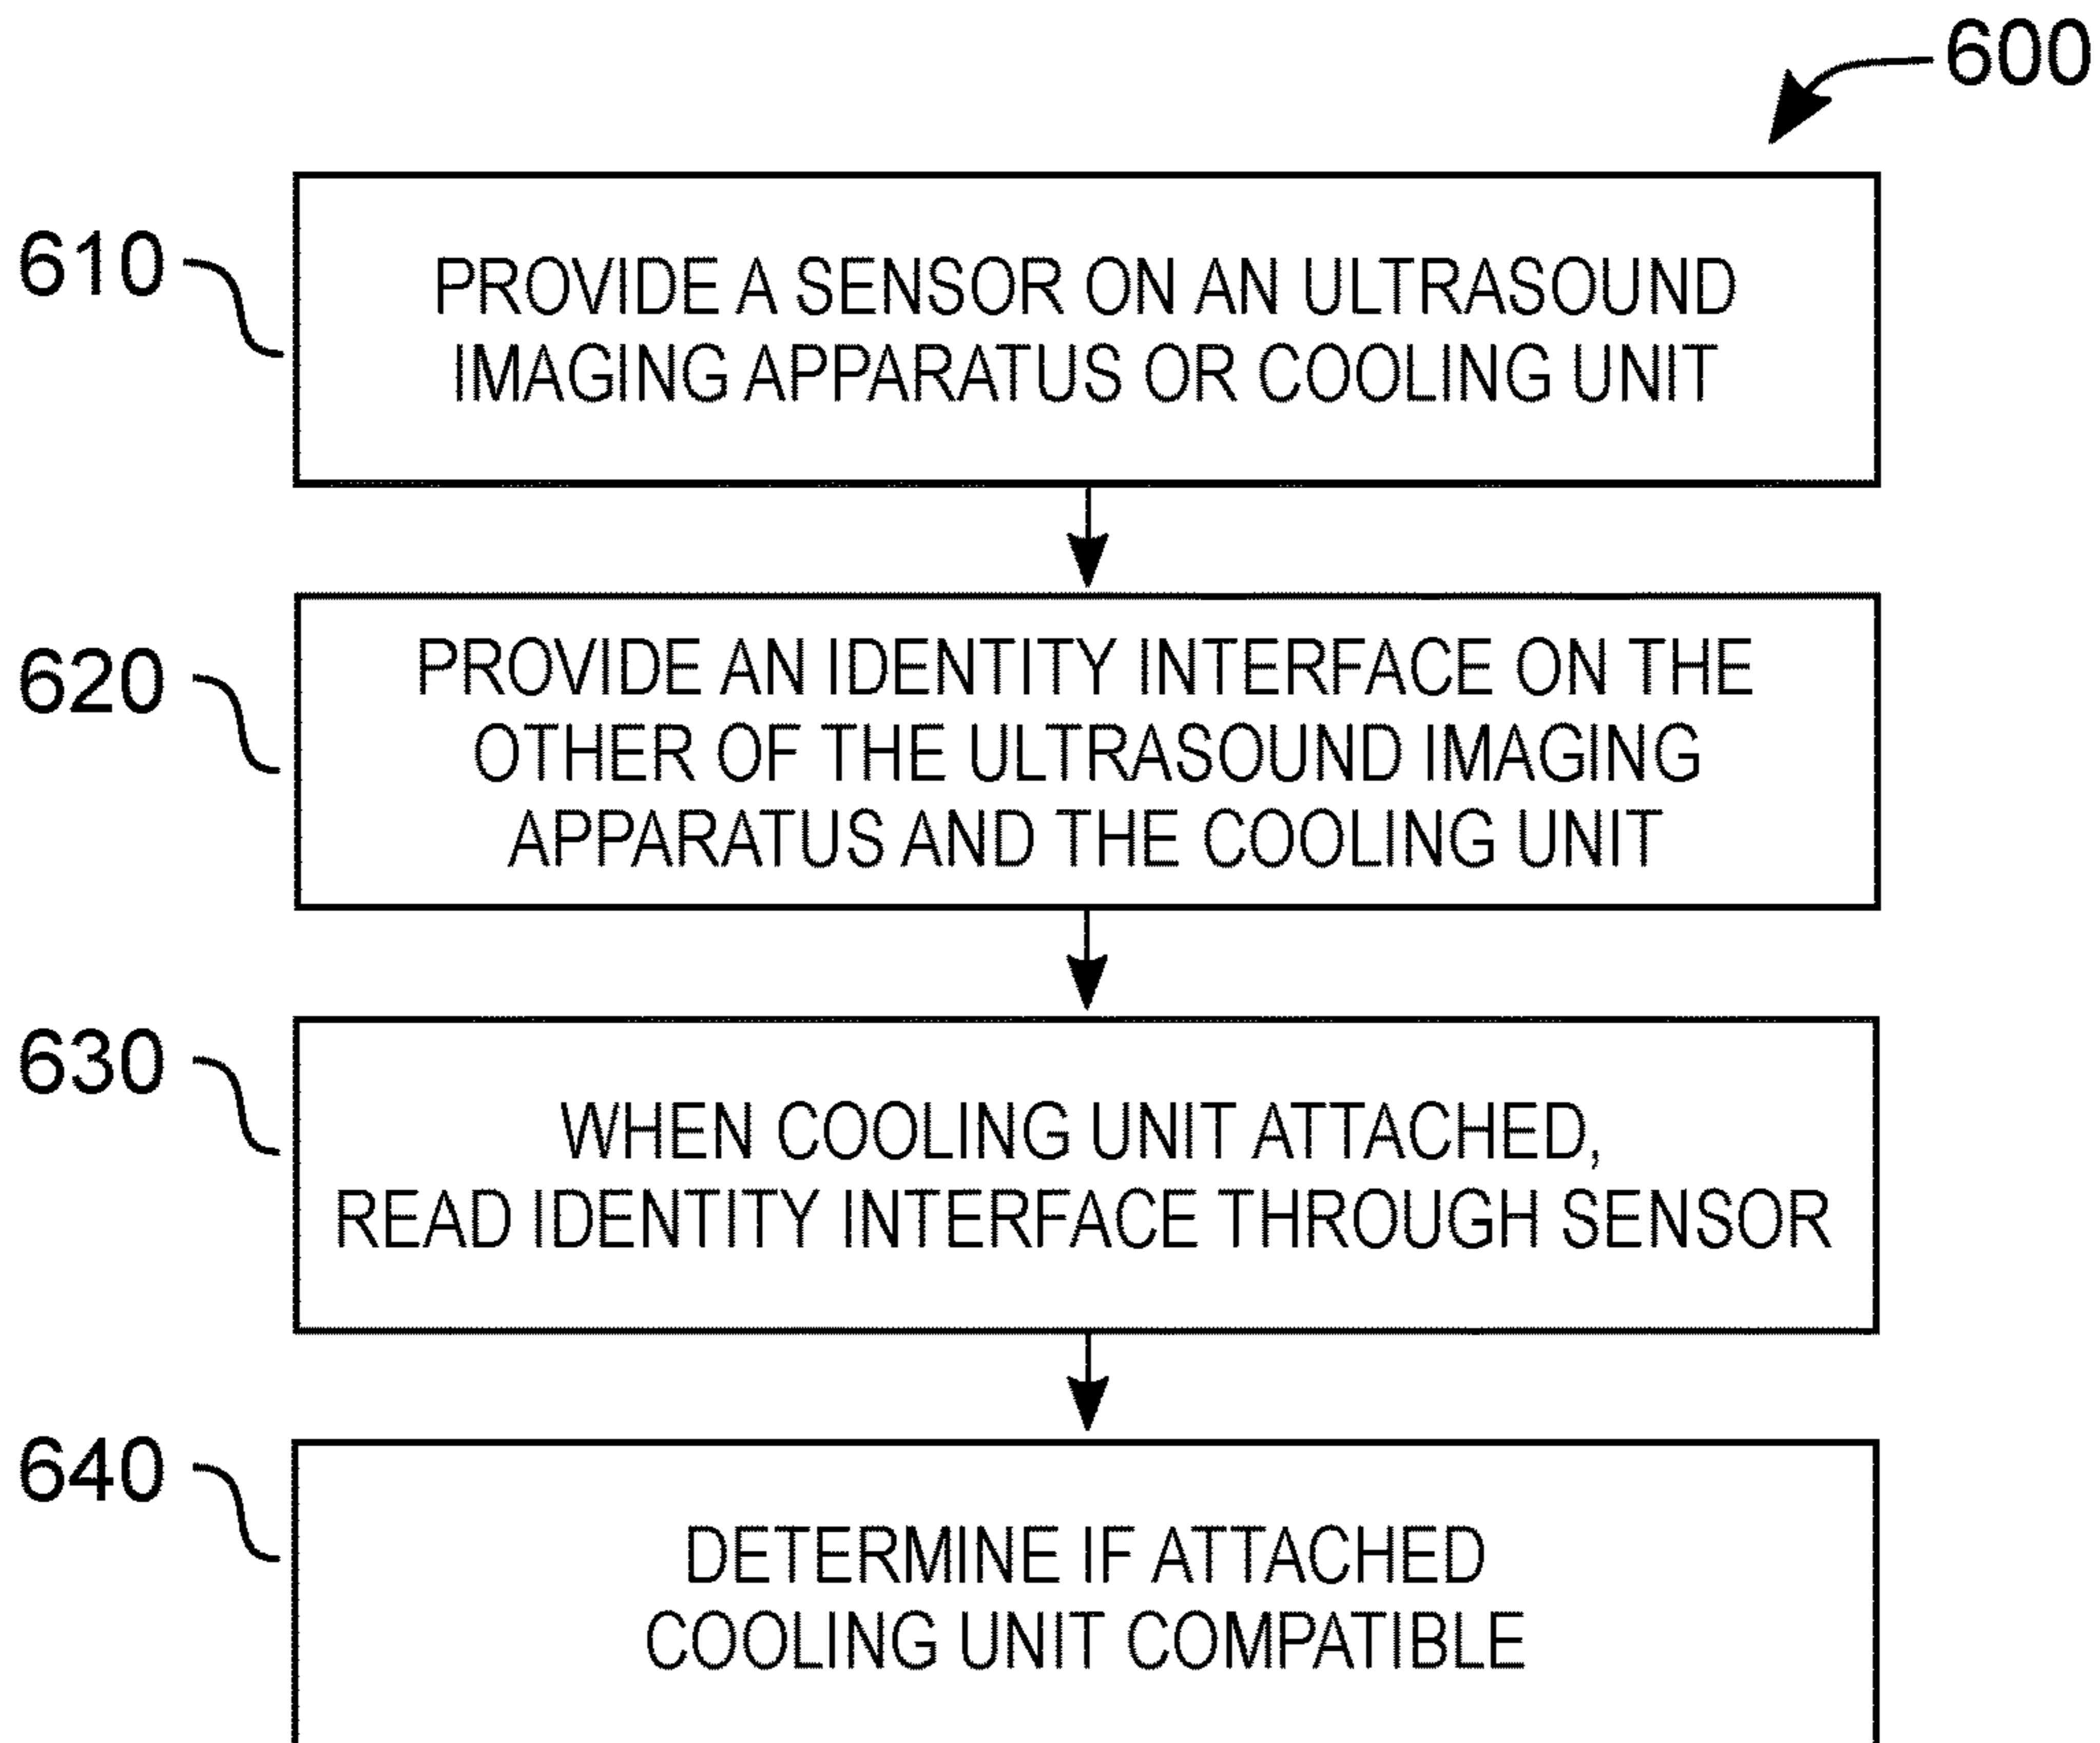


FIG. 6

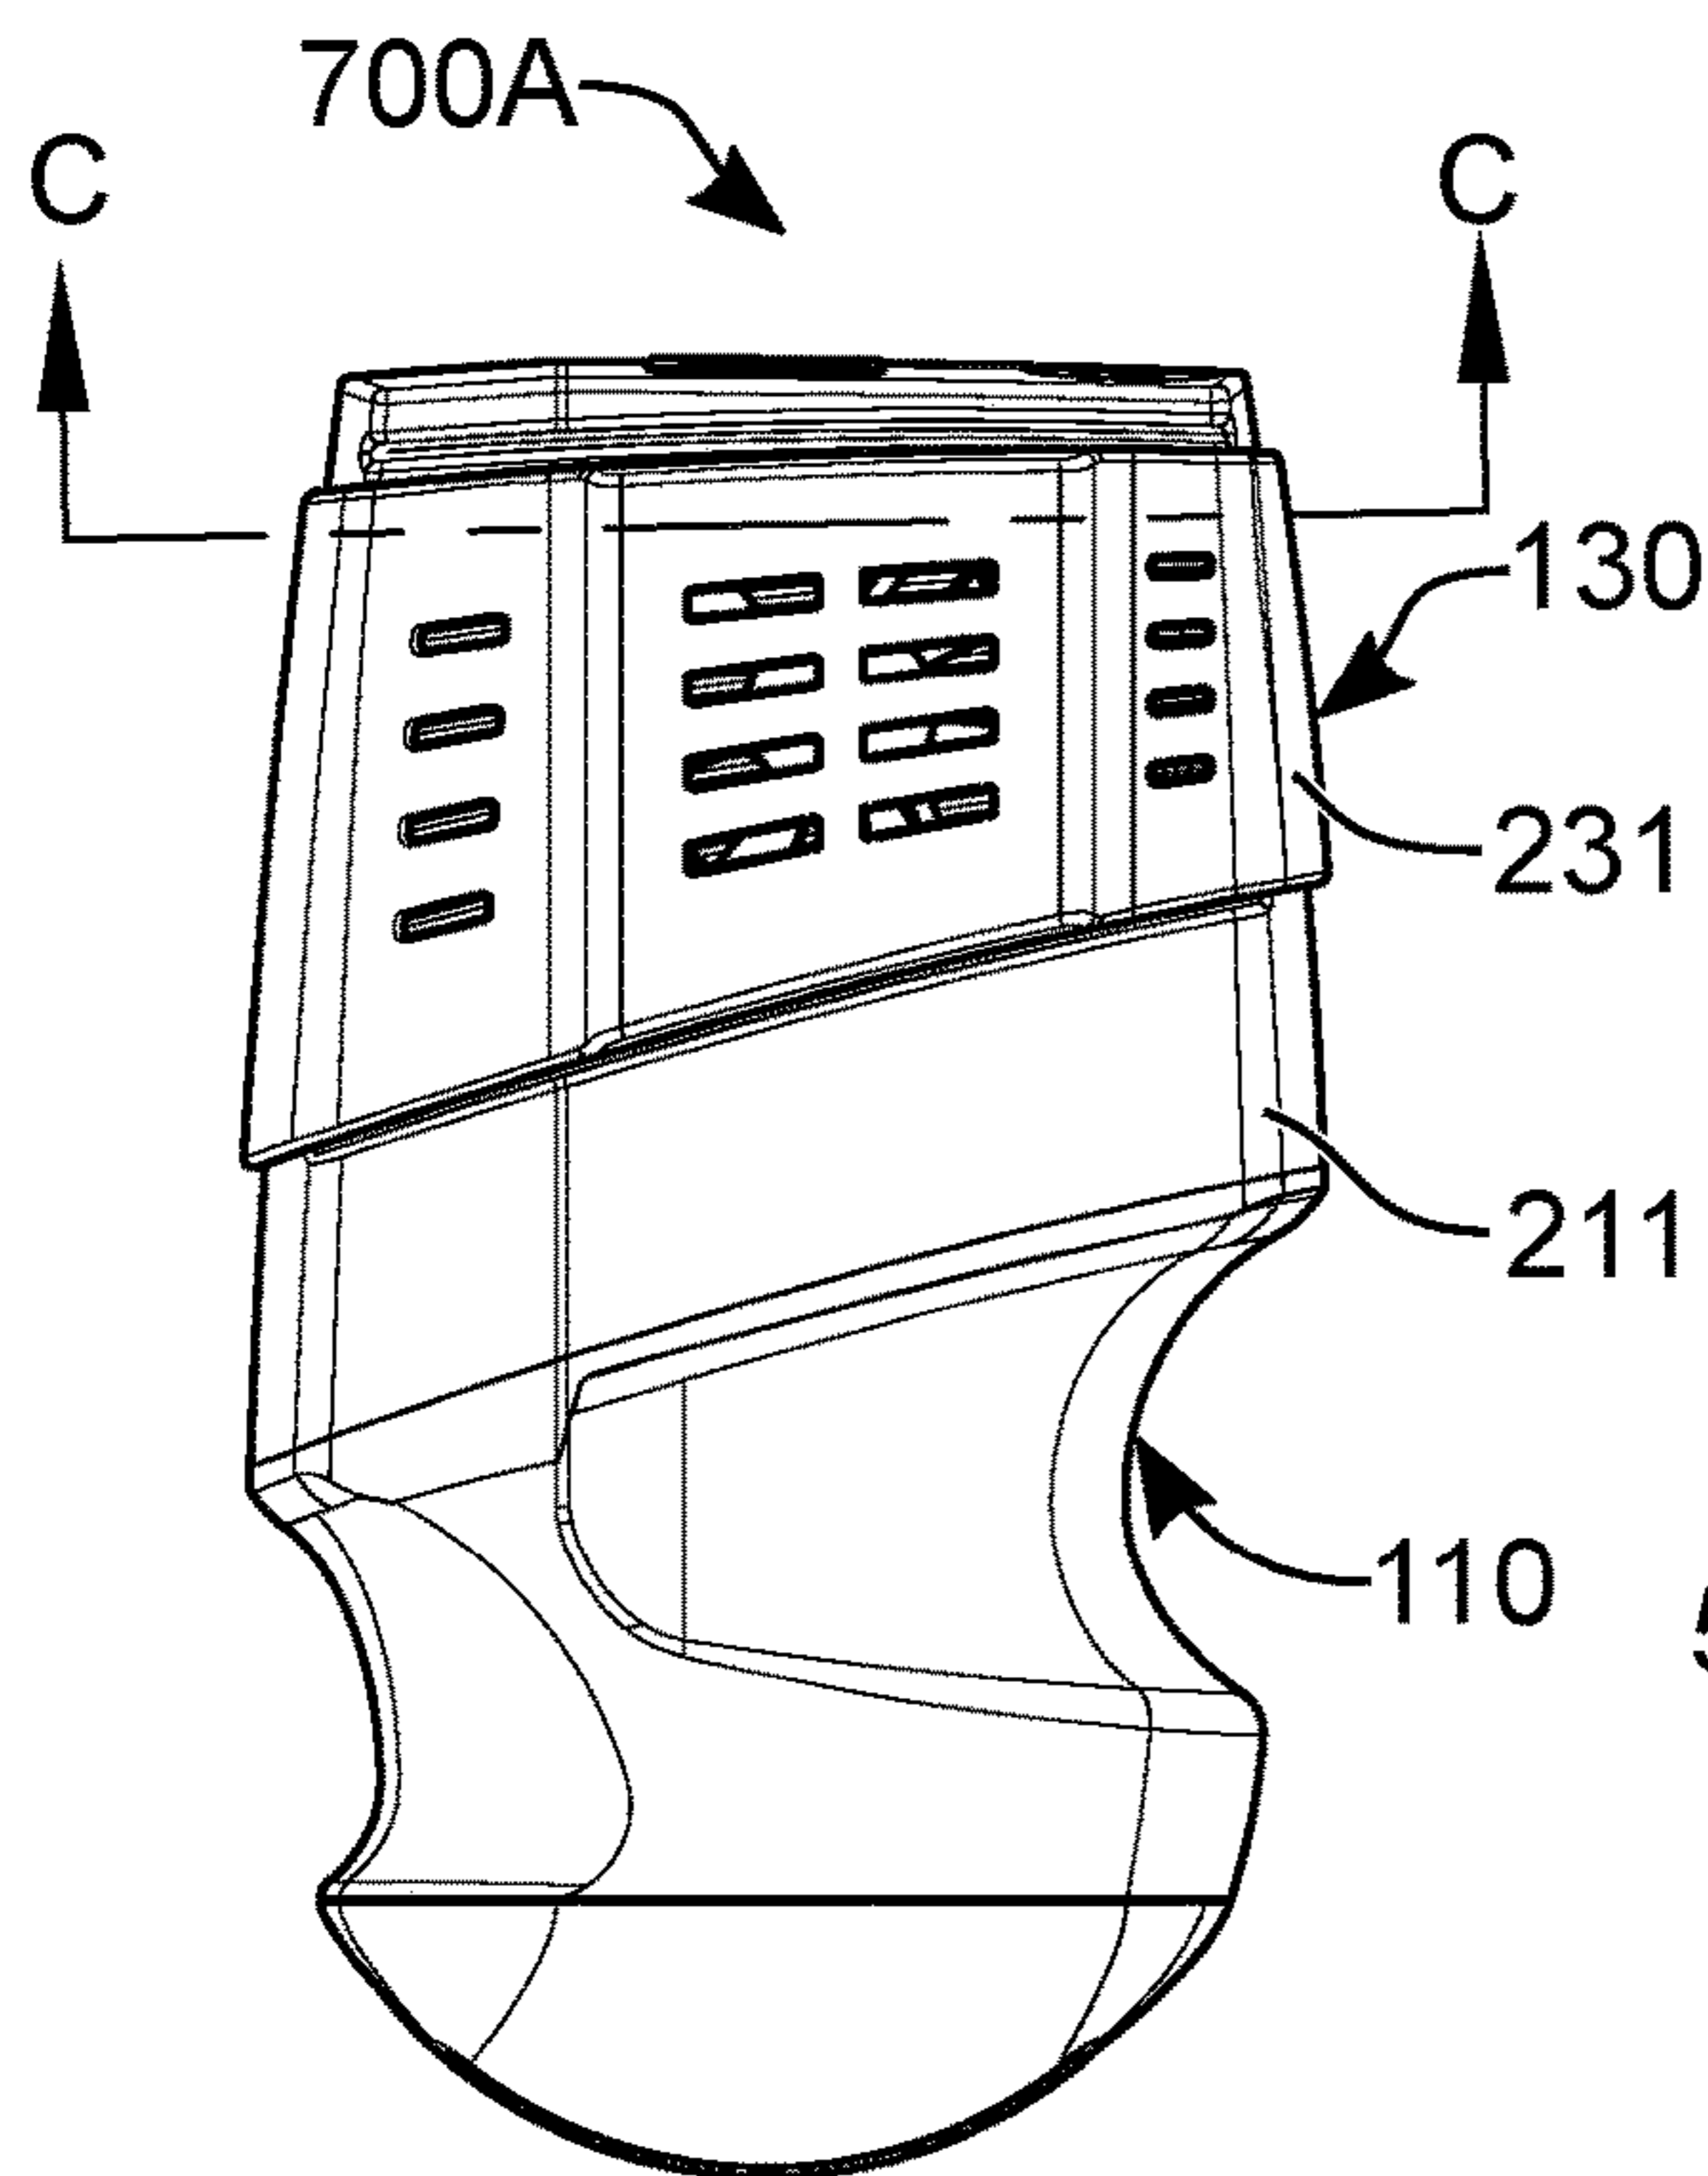


FIG. 7A

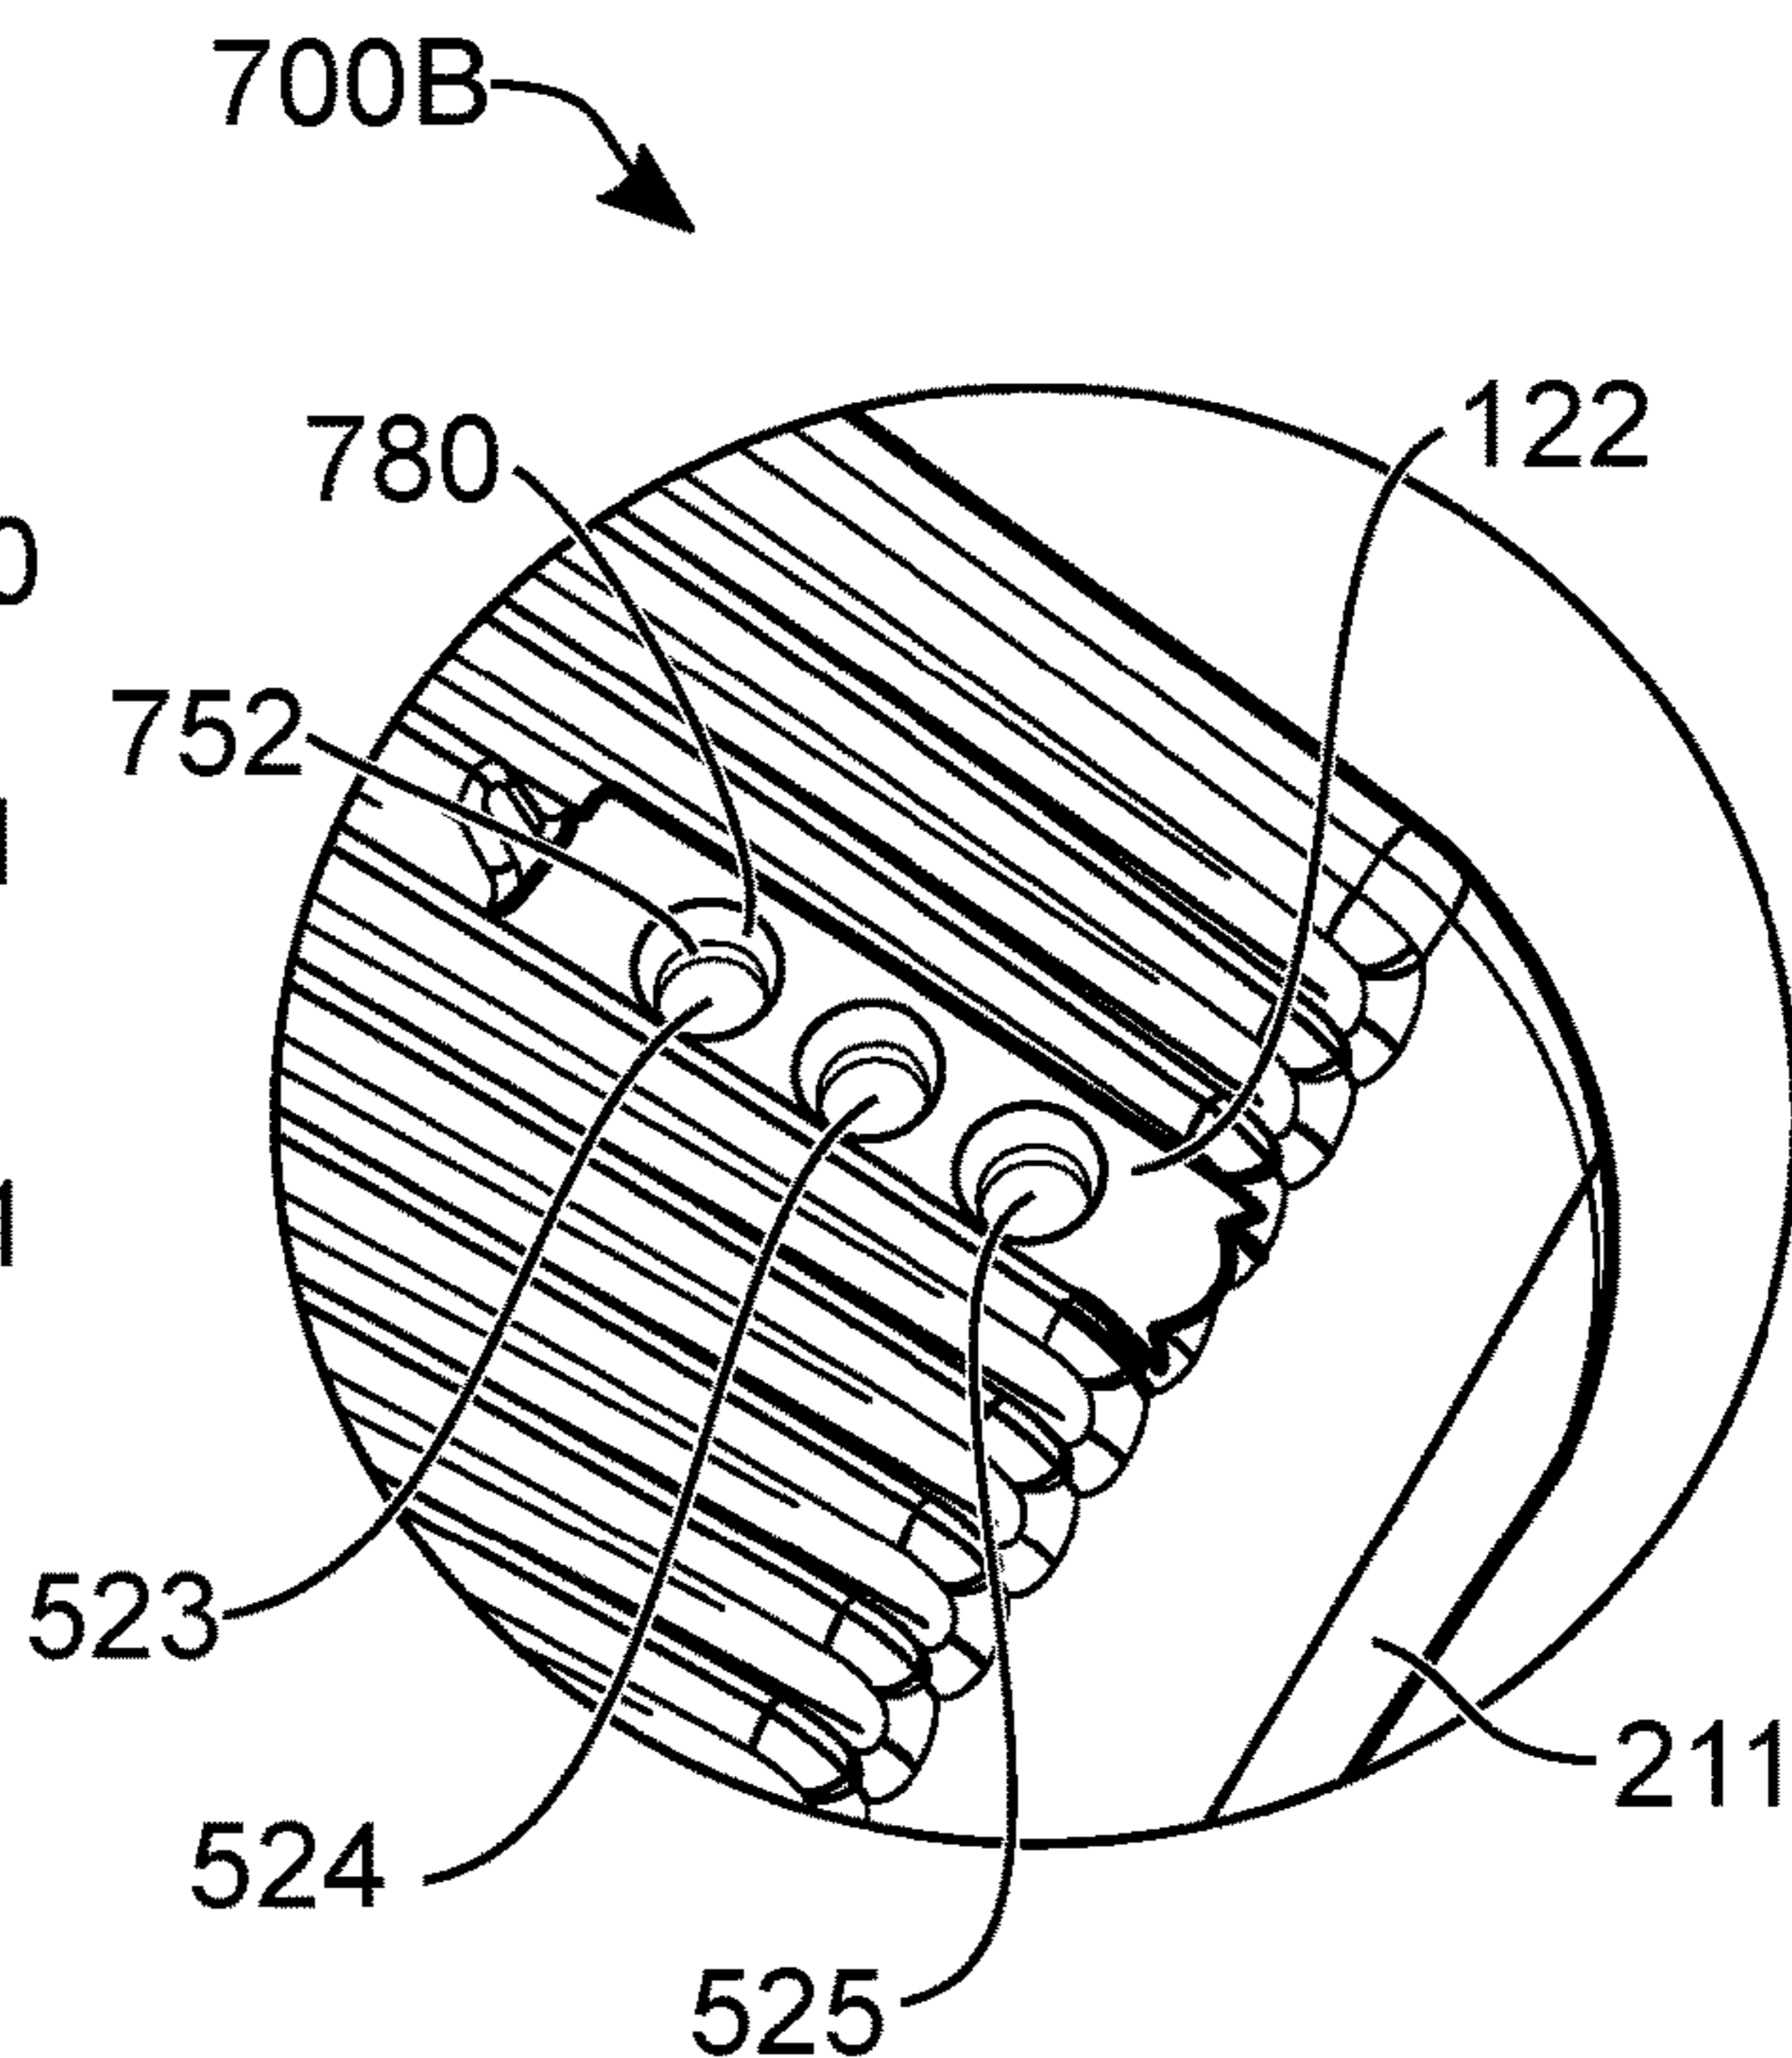


FIG. 7B

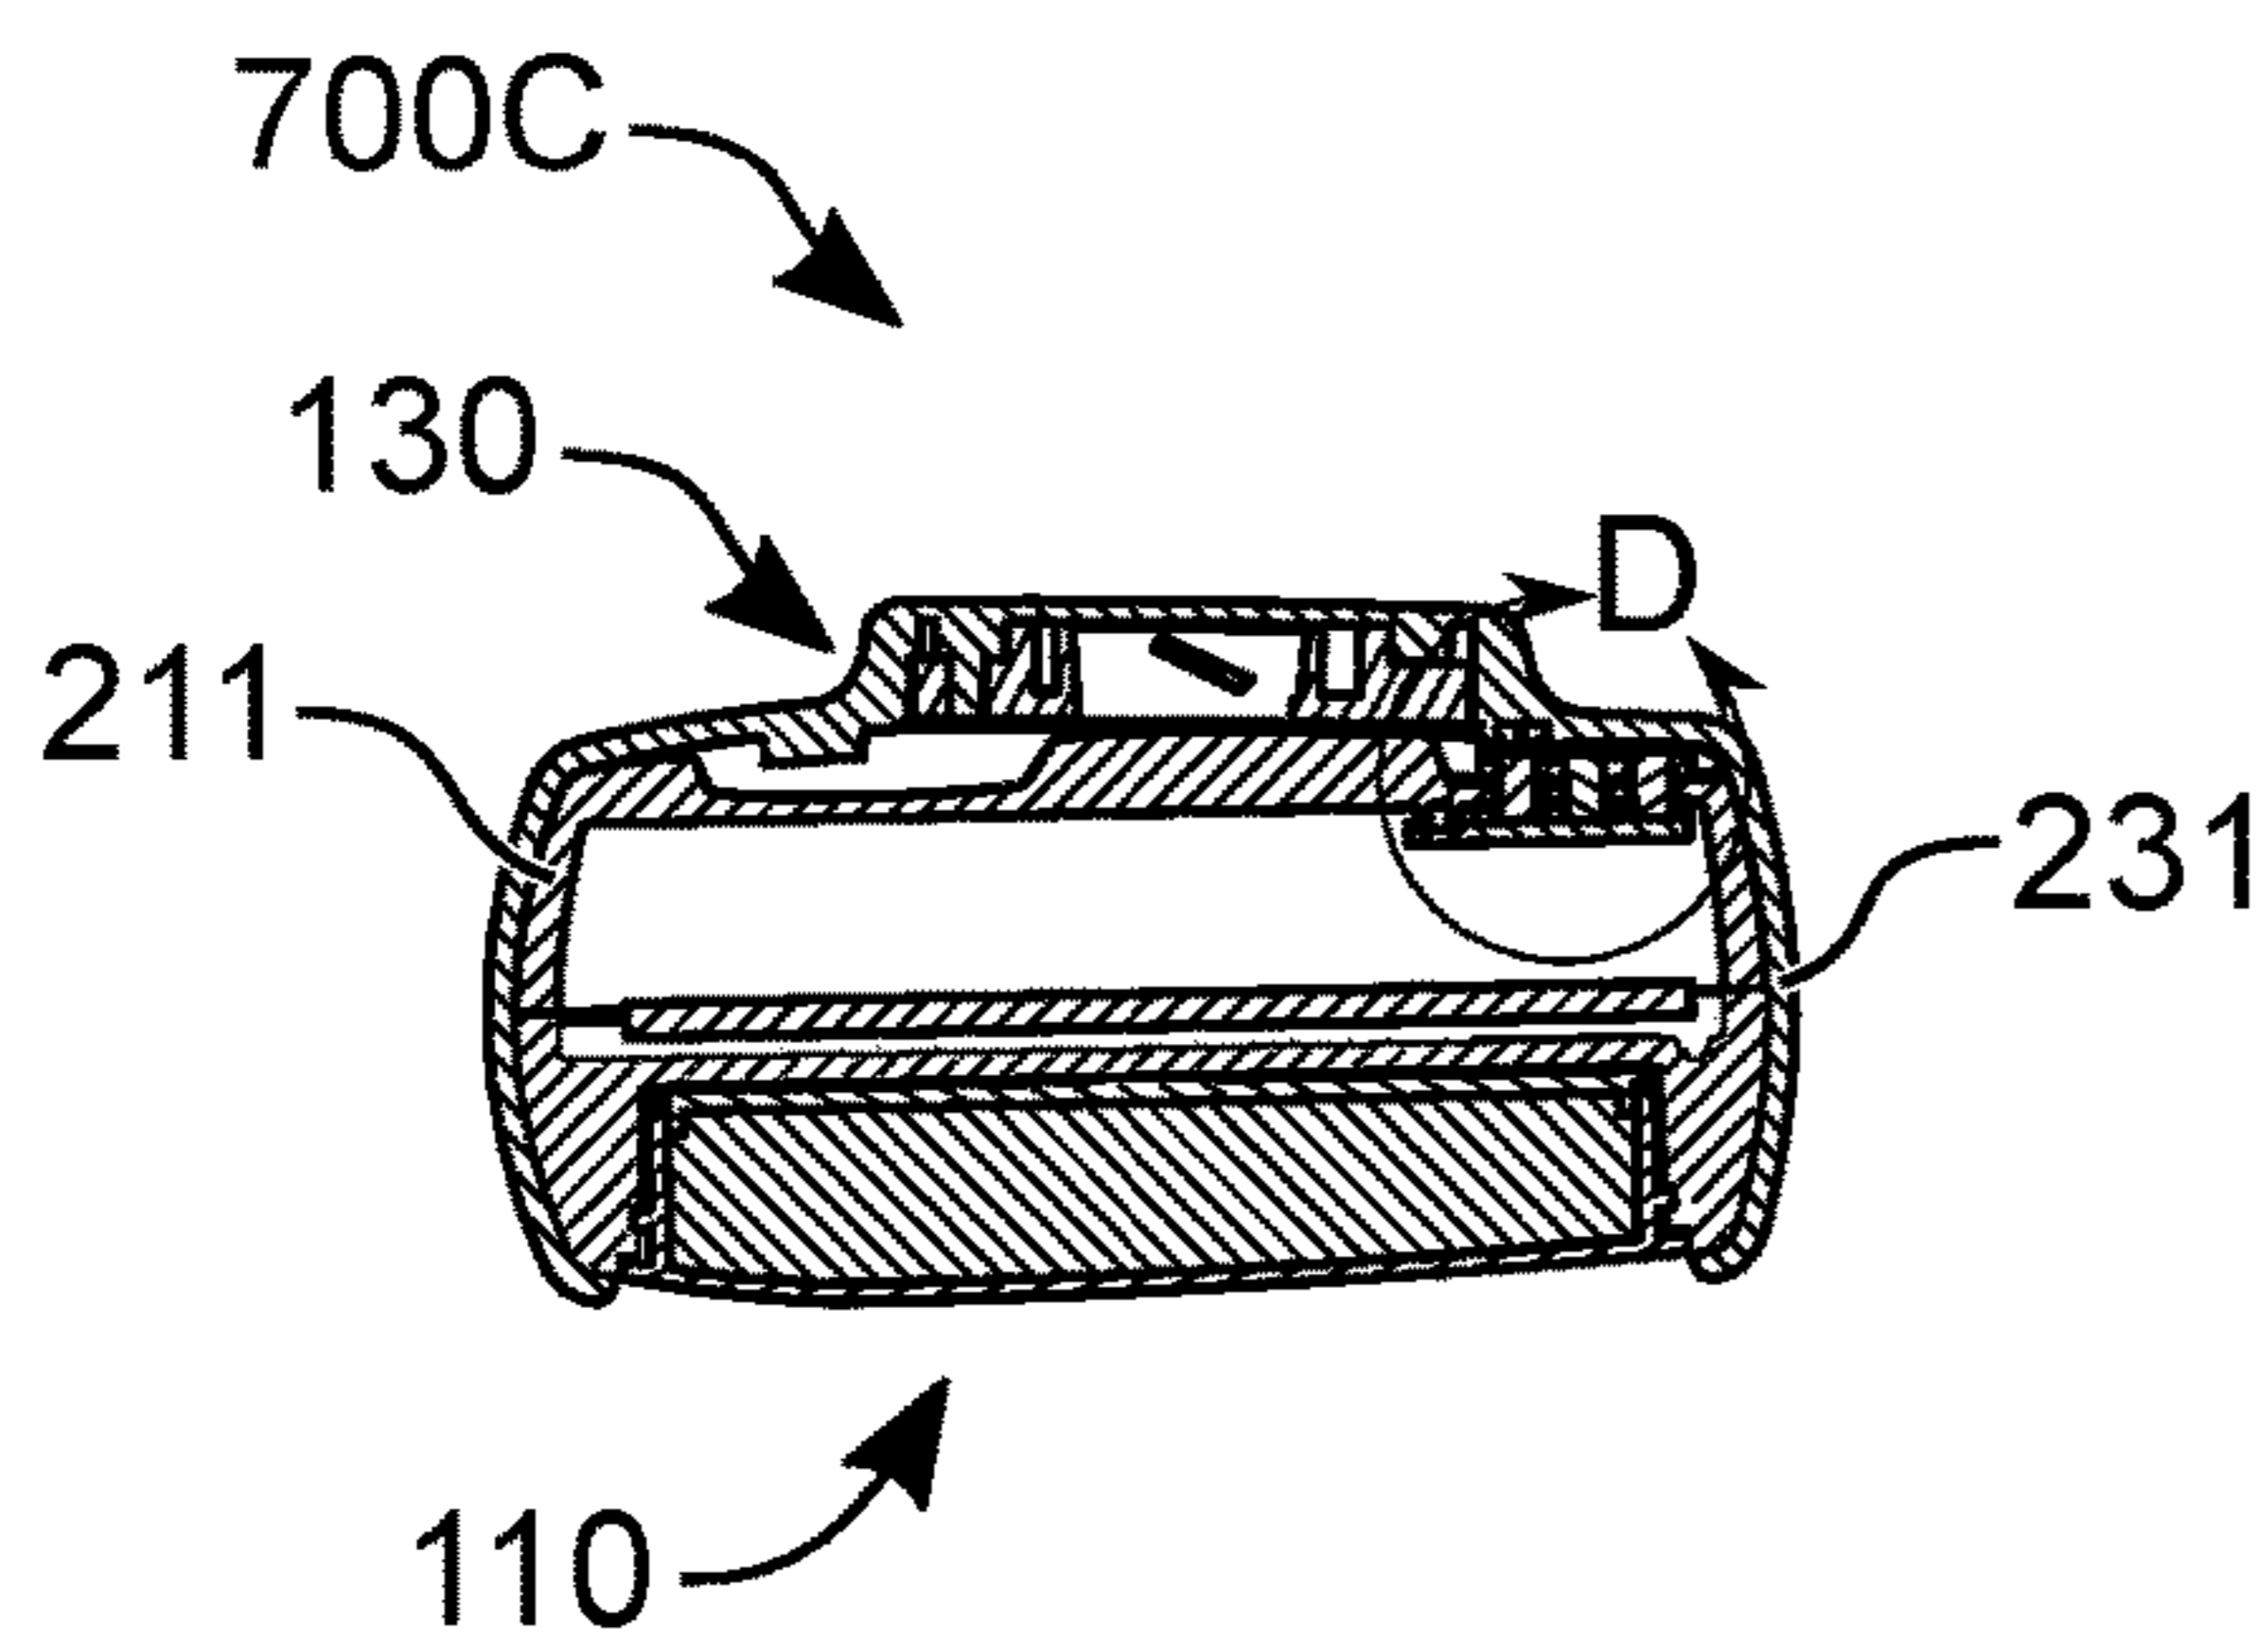


FIG. 7C

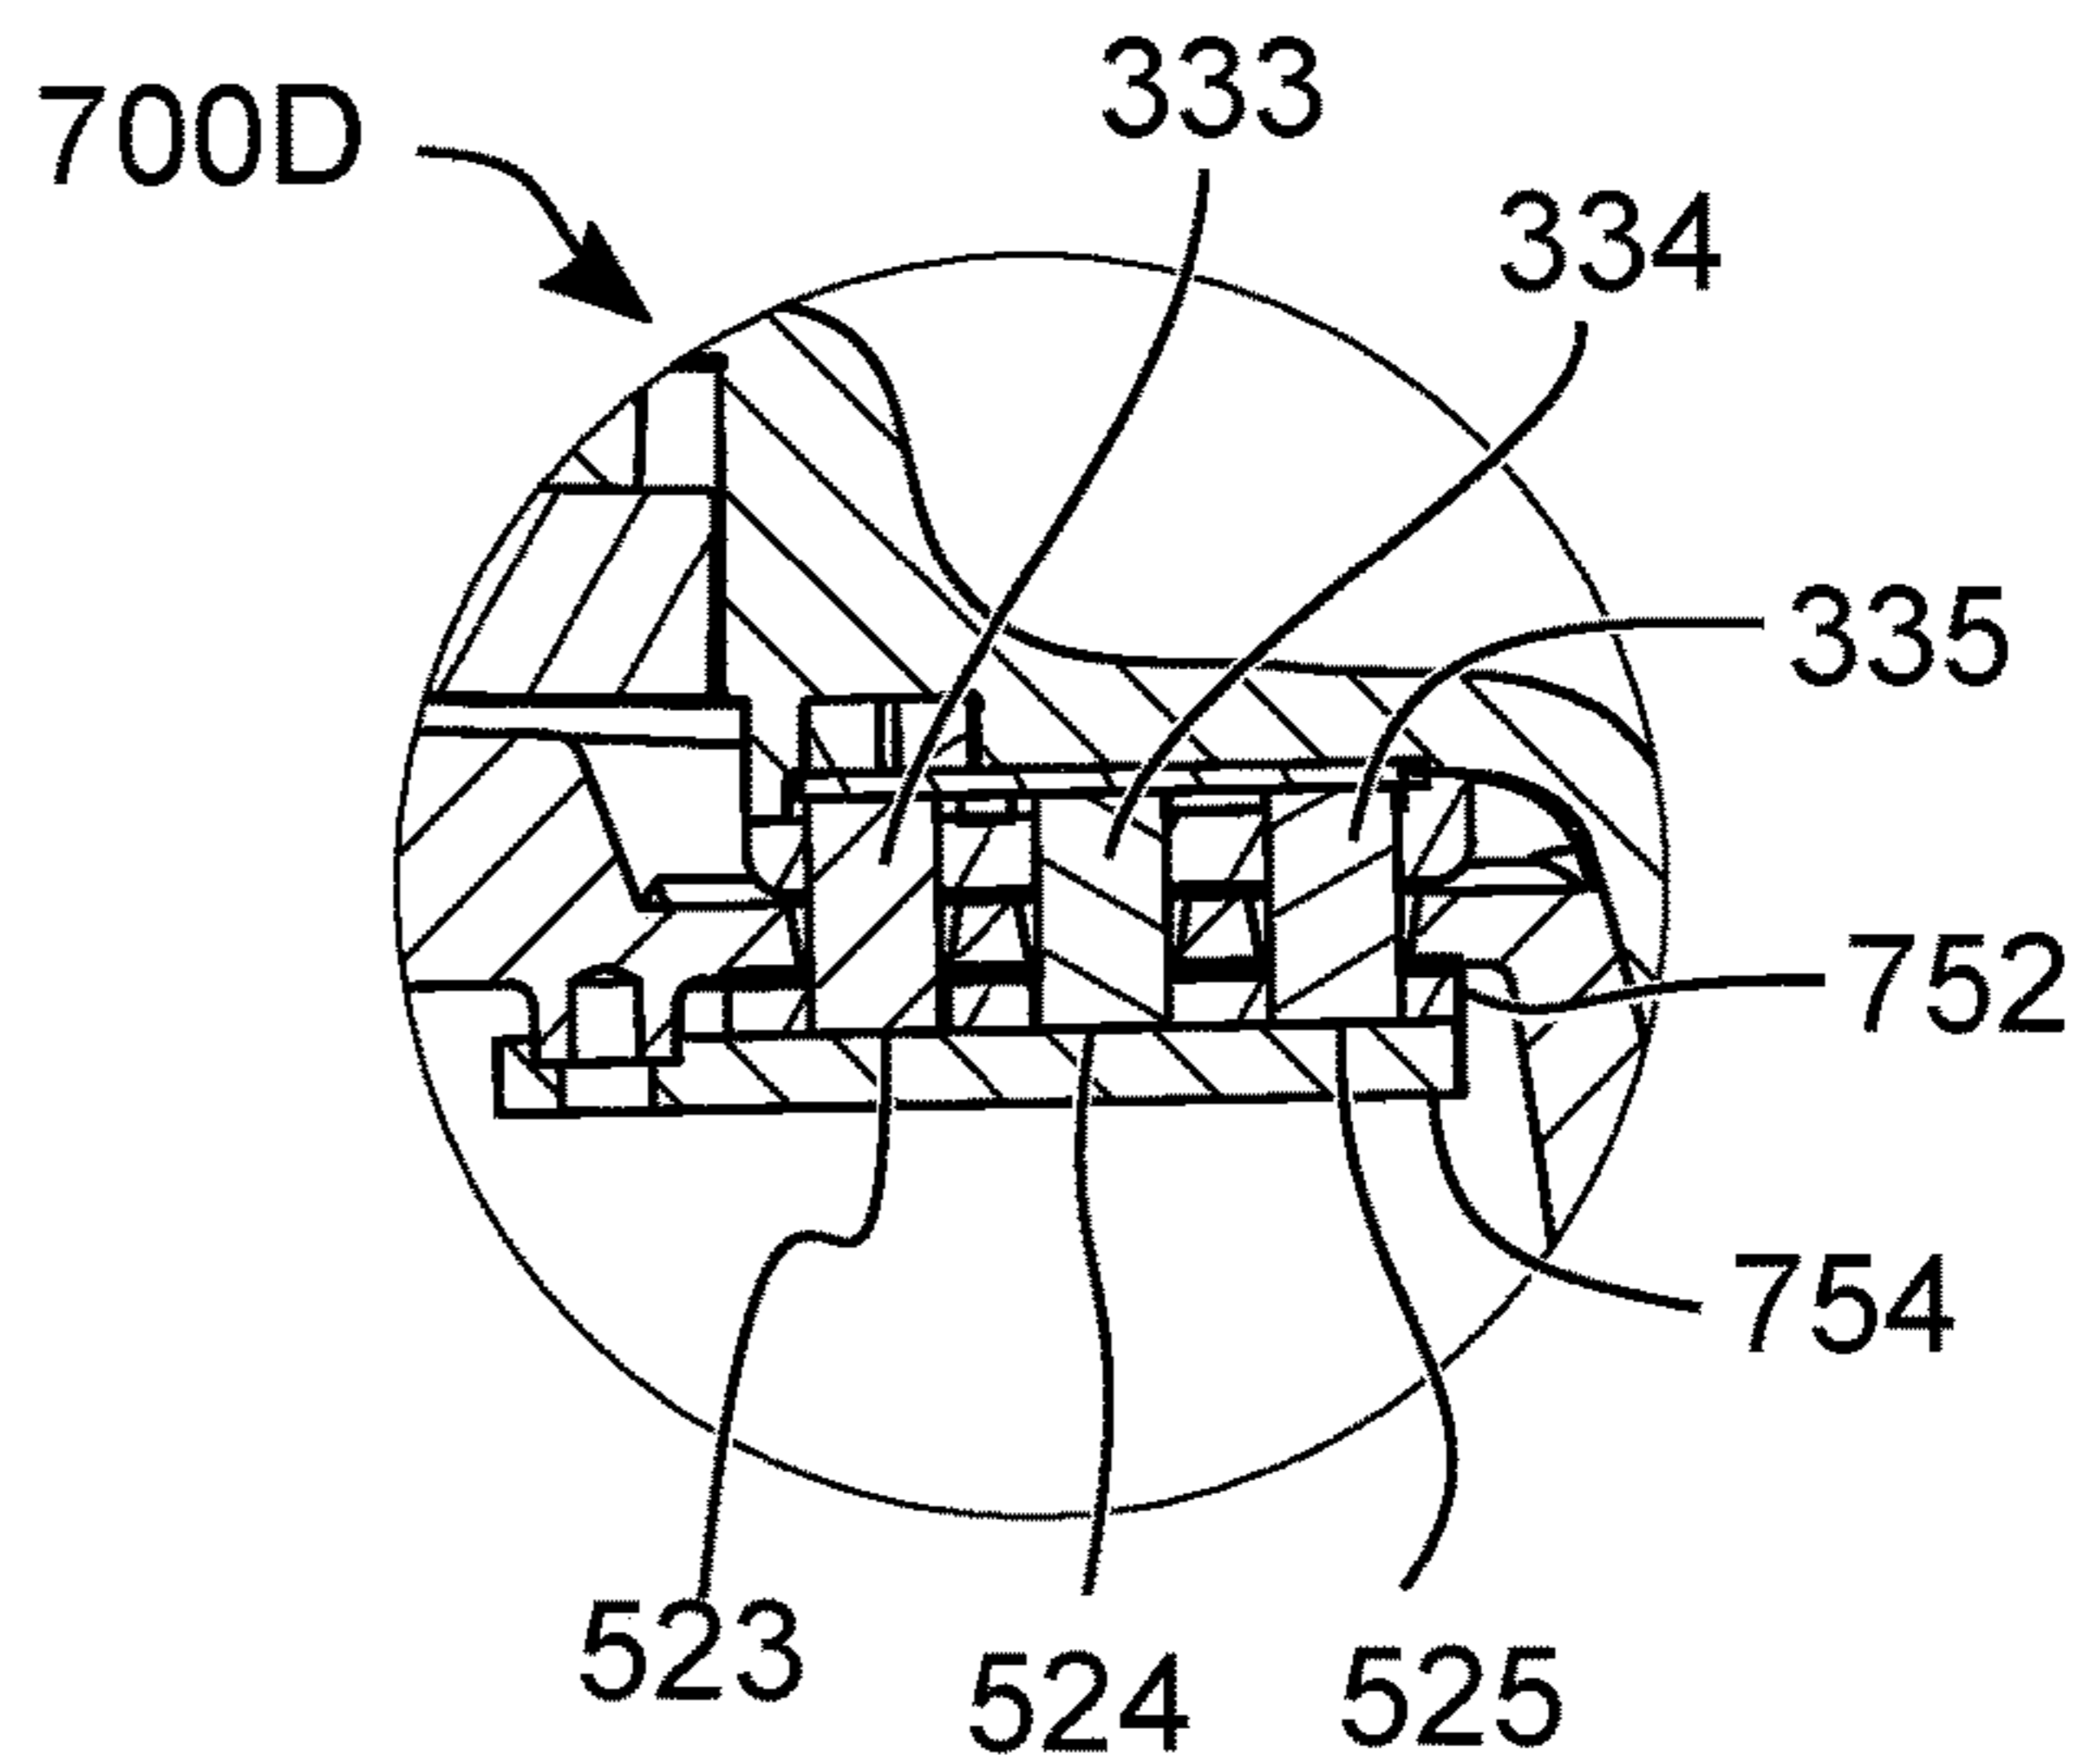


FIG. 7D

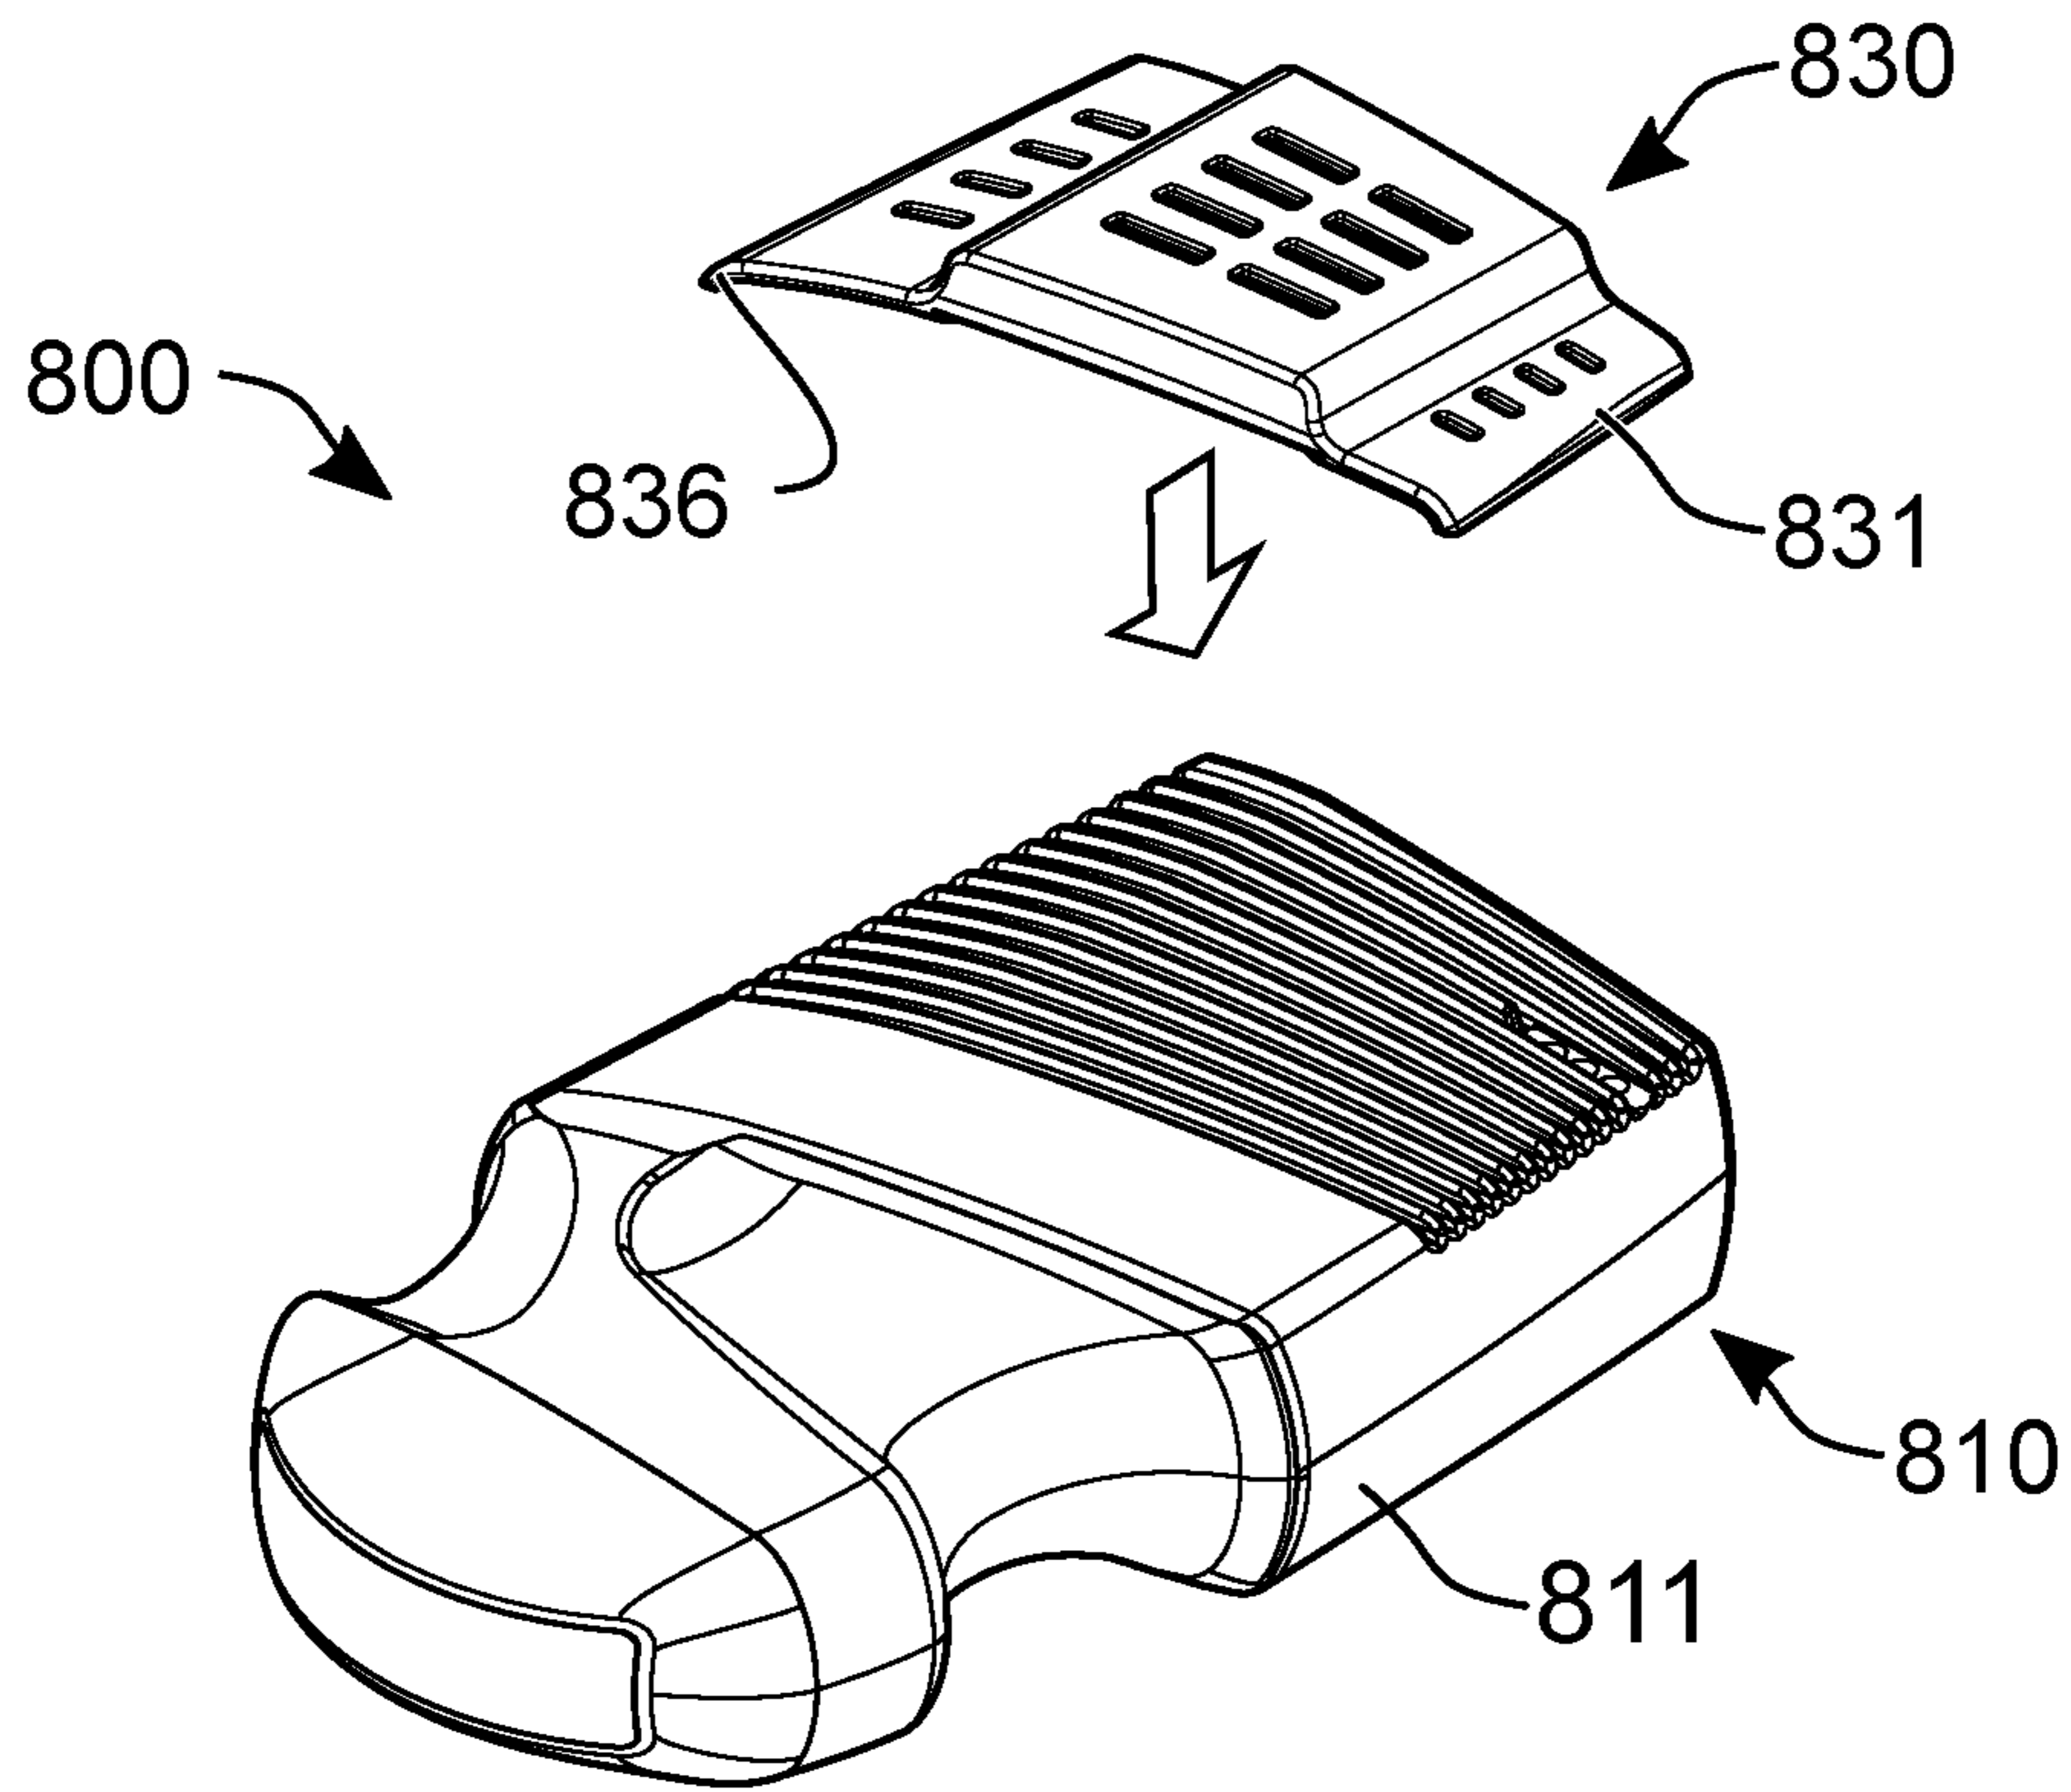


FIG. 8

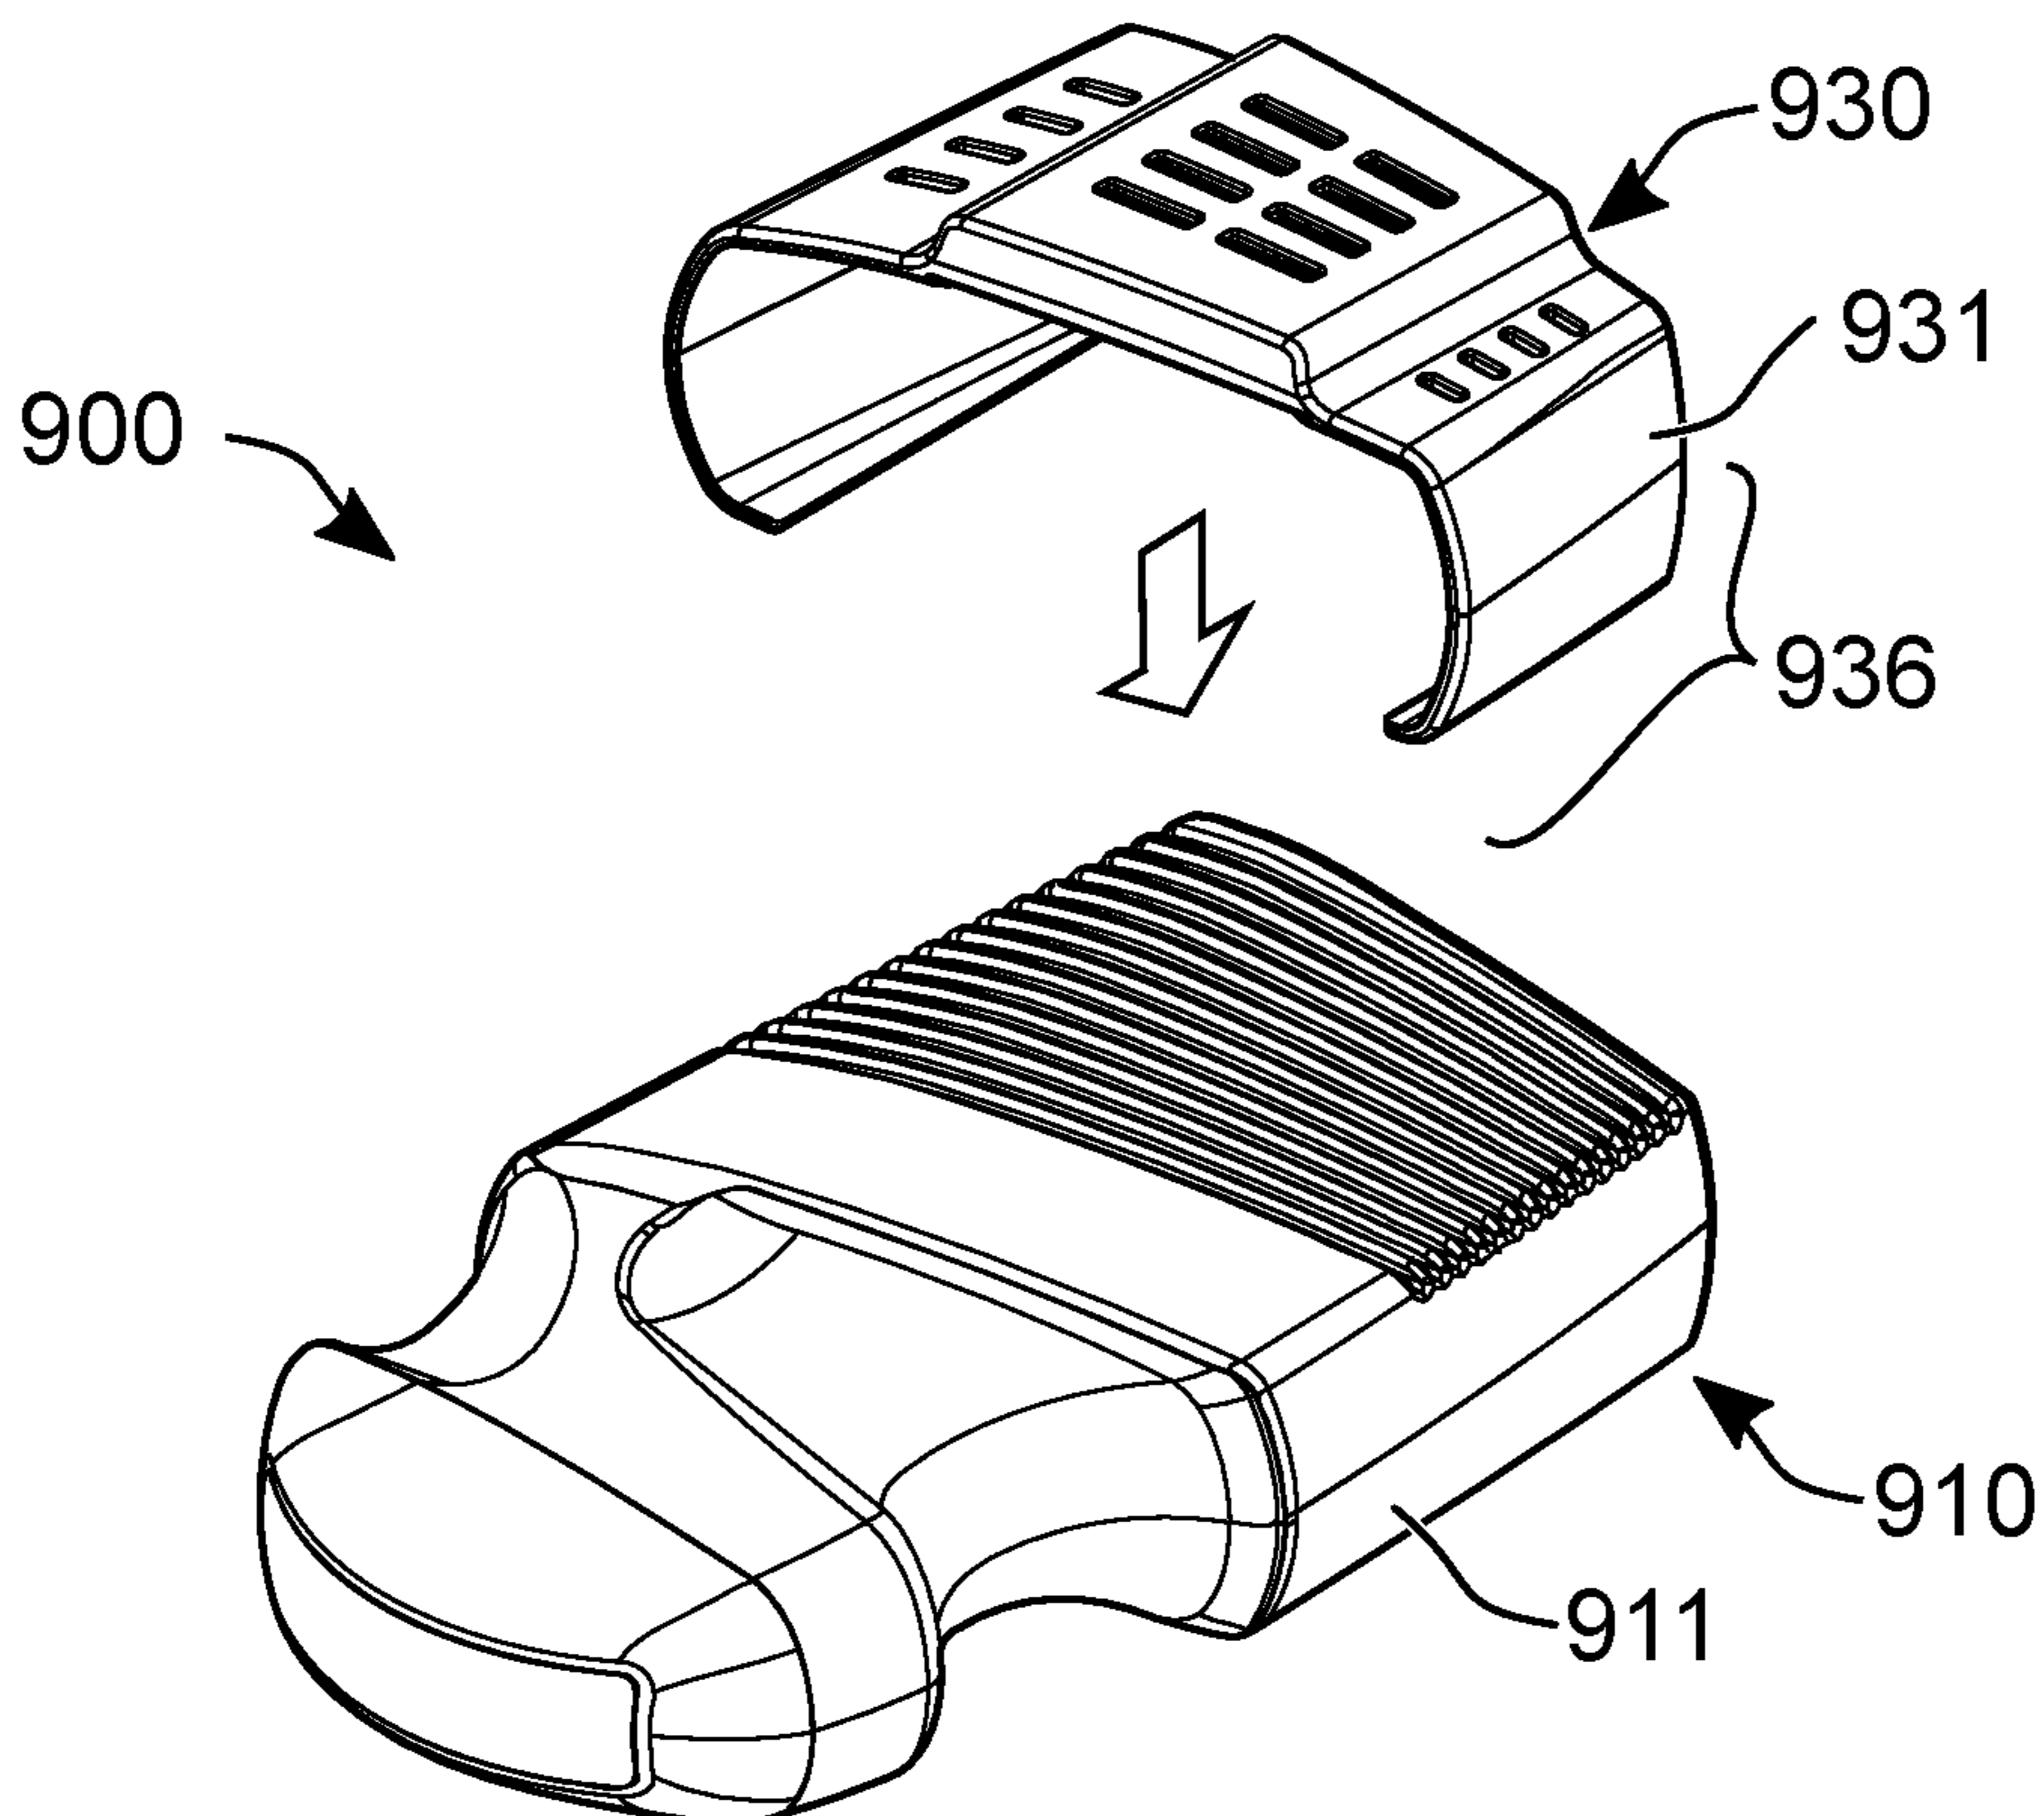


FIG. 9

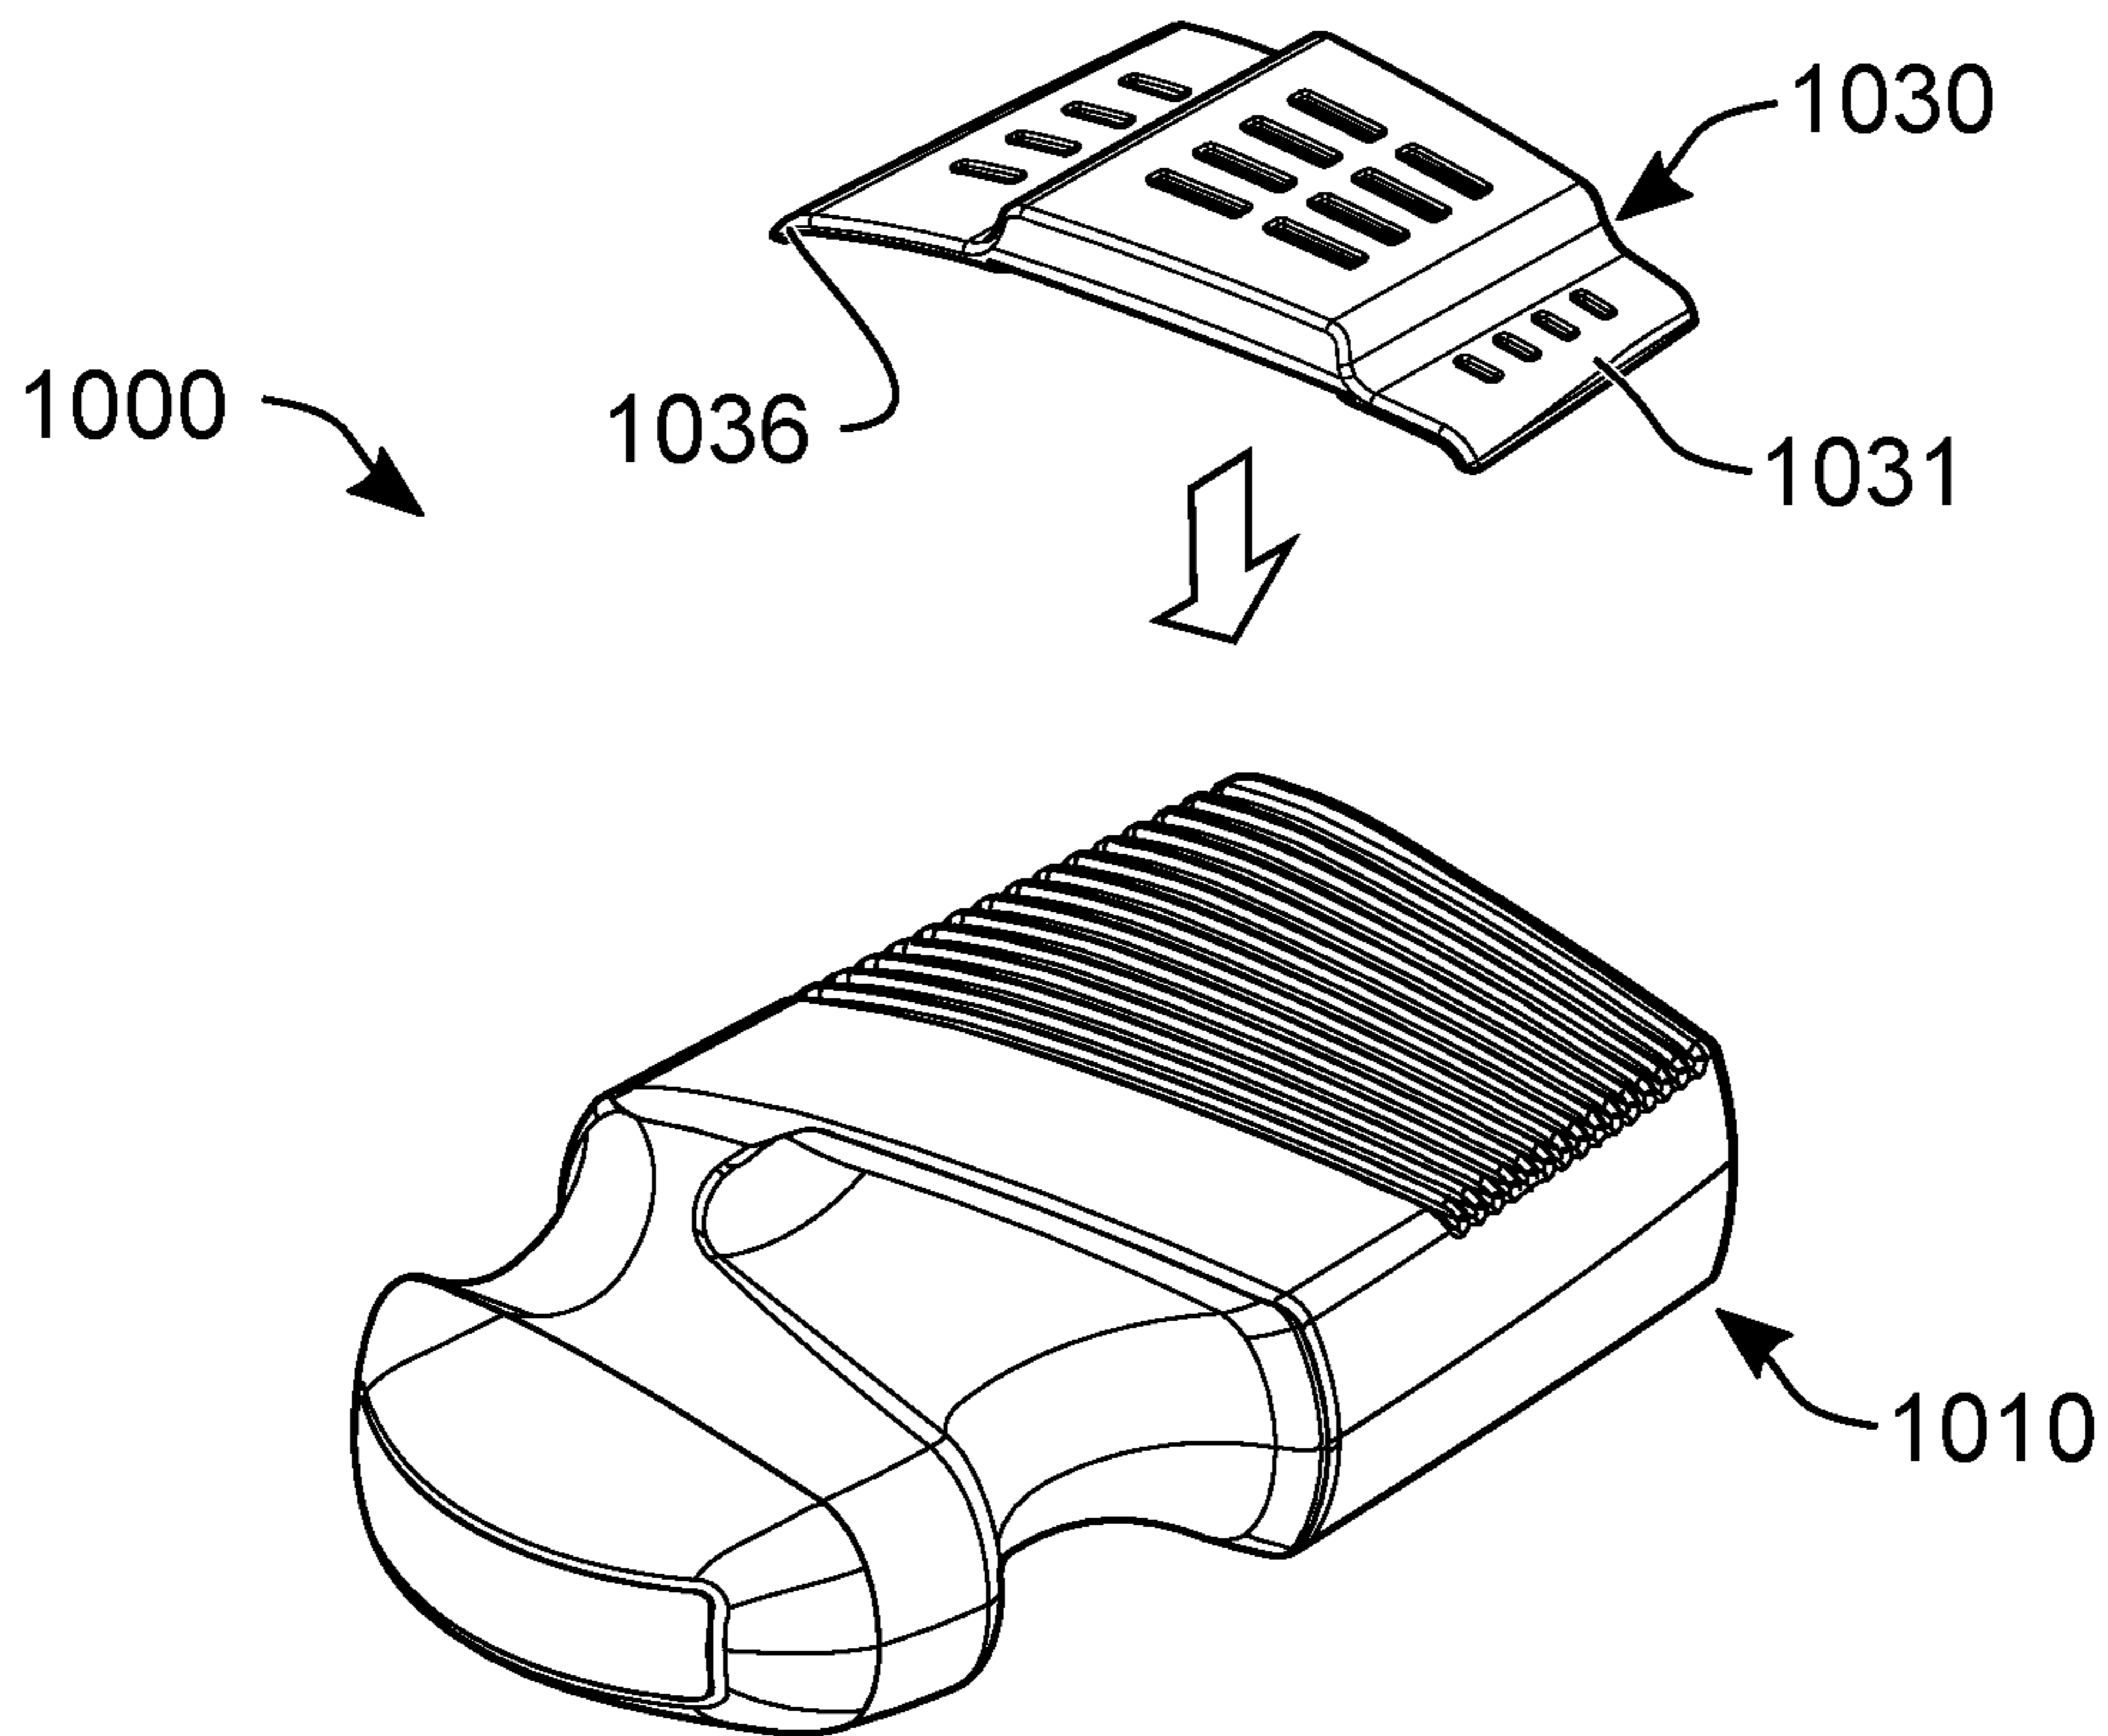


FIG. 10

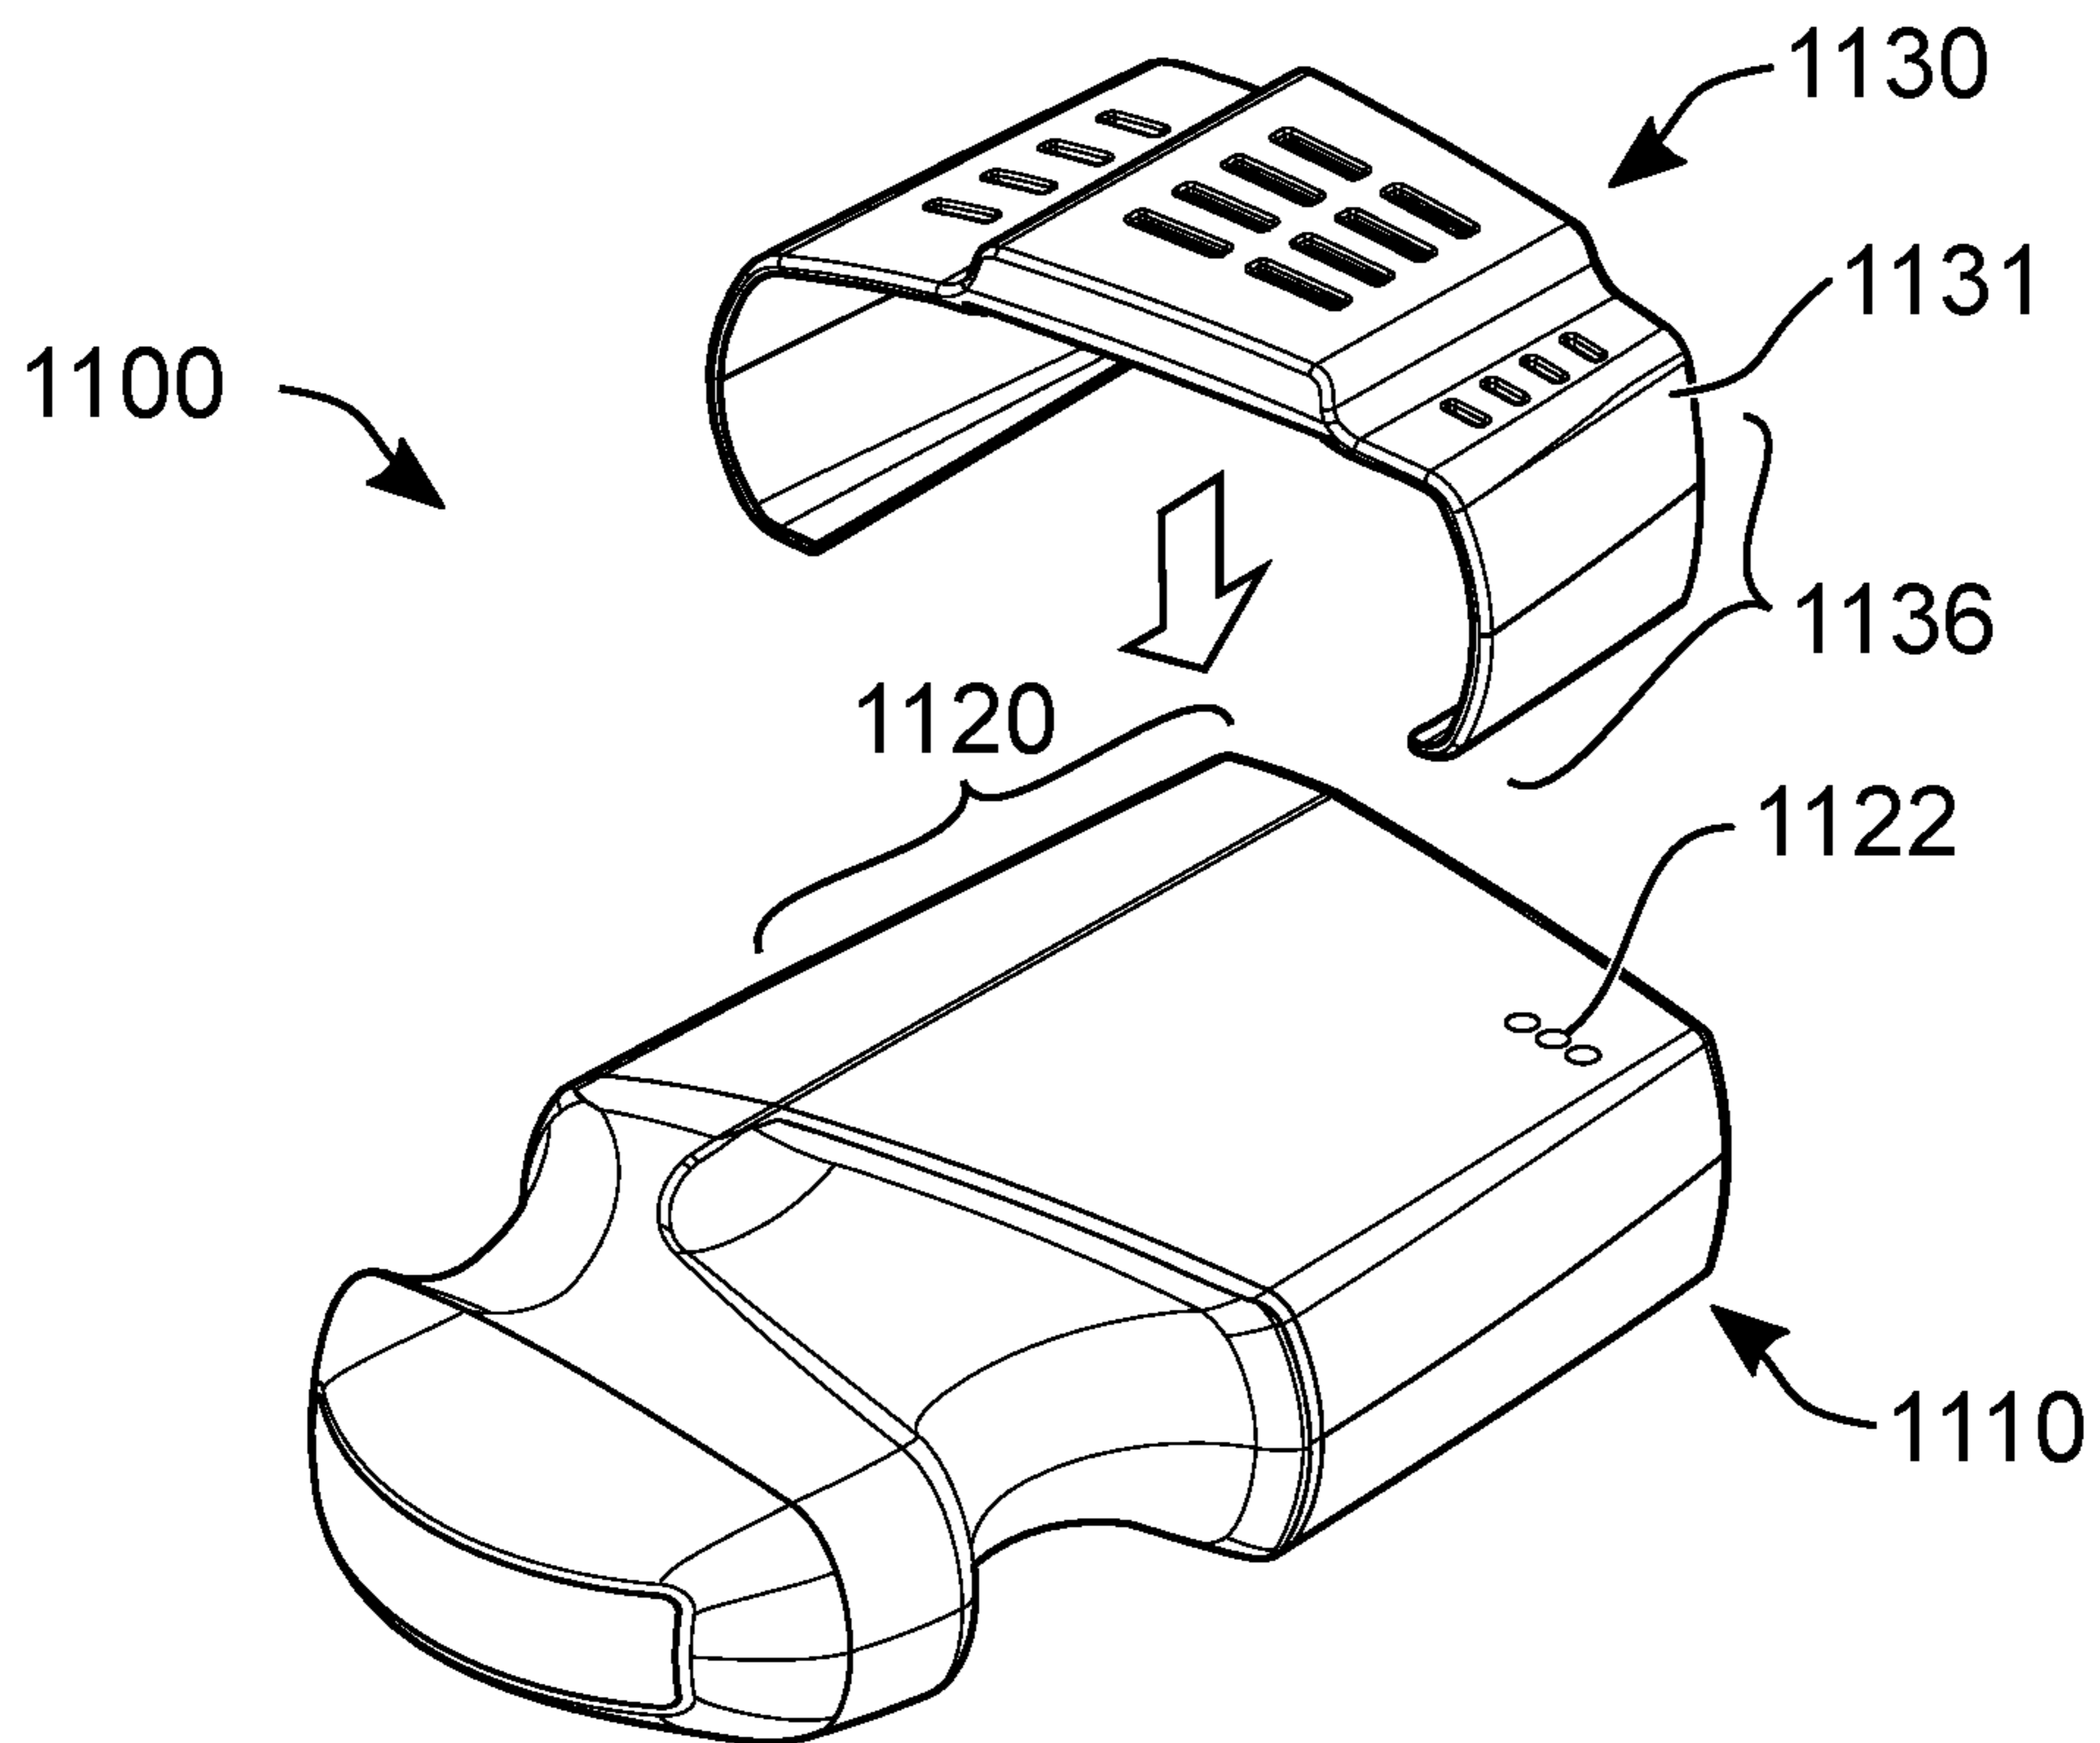


FIG. 11

COOLING UNIT FOR AN ULTRASOUND IMAGING APPARATUS, AND RELATED ULTRASOUND SYSTEMS

FIELD

The present disclosure relates generally to ultrasound imaging apparatus, and in particular, a cooling unit for an ultrasound imaging apparatus.

BACKGROUND

Ultrasound imaging systems may generate heat during operation. For example, heat may be generated from the transducer elements in a transducer array when they are activated to transmit ultrasound signals. Also, heat may be generated by integrated circuits (ICs) that drive the transducer array and process imaging data.

When imaging tissue, ultrasound probes (also called ultrasound transducers) are typically placed against the skin of a patient. To prevent patient injury or discomfort due to the probe head having overly high temperatures, there exist regulations that require surfaces of an ultrasound probe to not exceed certain predetermined temperatures while scanning a patient (e.g. International Electrotechnical Commission (IEC) standard 60601 requires external surfaces of an ultrasound probe to not exceed 48° C. in certain conditions).

There are traditional methods of dissipating heat from an ultrasound imaging apparatus. For example, in a traditional wired ultrasound system, heat may be channeled into and through the cable so that it can be dissipated from the cable and/or through the processing body. Heat may also traditionally be dissipated through conduction to the operator and to the patient, and/or through convection to the air. However, during lengthy periods of continuous scanning, these traditional heat mechanisms may not be sufficient.

In addition to adequate heat management, several other considerations may influence the design and operation of an ultrasound imaging apparatus; including ergonomics, battery life, and cleaning.

For example, in a wireless ultrasound imaging apparatus, it may be desirable to minimize the size and weight of the device; maximize operating time; and/or enable simple, quick, effective cleaning. A sealed and/or waterproof enclosure may, for example, enable easier cleaning and sterilization, and/or operation in wet environments. Some traditional wireless ultrasound systems include internal fans or other active cooling elements to increase heat dissipation. However, such traditional systems also typically include slits or vents in the housing to allow airflow caused by the fan. Such slits or vents may make it difficult to clean the ultrasound system without exposing the internal fan or electronics to cleaning fluid that may cause damage to those components.

There is thus a need for improved cooling mechanisms for ultrasound imaging apparatuses. The embodiments discussed herein may address and/or ameliorate at least some of the aforementioned design considerations identified above. The foregoing examples of the related art and limitations related thereto are intended to be illustrative and not exclusive. Other limitations of the related art will become apparent to those of skill in the art upon a reading of the specification and a study of the drawings herein.

BRIEF DESCRIPTION OF THE DRAWINGS

Non-limiting examples of various embodiments of the present disclosure will next be described in relation to the drawings, in which:

FIG. 1 shows a schematic representation of an ultrasound system, in accordance with at least one embodiment of the present invention;

FIG. 2A-2B shows a perspective view of an ultrasound imaging system with an active cooling unit in a detached state and an attached state, respectively, in accordance with at least one embodiment of the present invention;

FIG. 3 shows a rear perspective view of the active cooling unit of FIG. 2A-2B, in accordance with at least one embodiment of the present invention;

FIG. 4 shows a partial break-out section view of the ultrasound imaging system when the cooling unit is attached, in accordance with at least one embodiment of the present invention;

FIG. 5 shows an electrical schematic of some of the components of the ultrasound imaging system of FIG. 2A-2B, in accordance with at least one embodiment of the present invention;

FIG. 6 is a flowchart diagram showing steps of a method for determining whether an active cooling unit is attached to and compatible with an ultrasound imaging apparatus, in accordance with at least one embodiment of the present invention;

FIG. 7A shows a front view of the ultrasound imaging system of FIGS. 2A-2B, in accordance with at least one embodiment of the present invention;

FIG. 7B shows an enlarged partial perspective view of the connector of the ultrasound imaging apparatus of FIGS. 2A-2B, in accordance with at least one embodiment of the present invention;

FIG. 7C shows a cross-sectional view of the ultrasound imaging system of FIG. 2A-2B along line C-C shown in FIG. 7A, in accordance with at least one embodiment of the present invention;

FIG. 7D shows a detail view drawn from FIG. 7C of the ultrasound imaging system of FIG. 2A-2B, in accordance with at least one embodiment of the present invention; and

FIGS. 8-11 show perspective views of various alternative configurations of an ultrasound imaging system, in accordance with various embodiments of the present invention.

DETAILED DESCRIPTION

In a first broad aspect of the present disclosure, there is provided an ultrasound imaging system, including: an ultrasound imaging apparatus operable to acquire ultrasound image data; and a cooling unit configured to be detachably coupled to the ultrasound imaging apparatus; wherein the cooling unit includes an active cooling element for removing heat from the ultrasound imaging apparatus, and wherein the cooling unit is cordless.

In some embodiments, the ultrasound imaging apparatus includes a sensor for detecting when the cooling unit is attached. In some embodiments, the sensor includes at least a portion of a resistor network. In some embodiments, the resistor network includes a resistor voltage divider network.

In some embodiments, the ultrasound imaging apparatus includes an external surface and the active cooling element includes a fan, and said fan is configured to direct air onto and/or from said external surface.

In some embodiments, the cooling unit includes at least one fastener to perform the detachable coupling. In some embodiments, the fastener is formed with a housing of the cooling unit. In some embodiments, the housing includes at least one clip portion to provide the detachable coupling.

In some embodiments, the cooling unit is coupled to the ultrasound imaging apparatus using magnetic force. In some

3

embodiments, the cooling unit includes a housing and said housing includes at least one magnet for performing the detachable coupling and wherein a body of the ultrasound imaging apparatus includes a magnetic material for mating with said at least one magnet.

In some embodiments, the ultrasound imaging apparatus provides power to the cooling unit. In some embodiments, the ultrasound imaging apparatus and the cooling unit include connectors configured to mate with one another. In some embodiments, the cooling unit receives power from the ultrasound imaging apparatus.

In some embodiments, the cooling unit is powered independently. In some embodiments, the cooling unit includes a battery for powering the active cooling element.

In some embodiments, the ultrasound imaging apparatus includes a shell, and wherein said shell protects from ingress into an interior of the ultrasound imaging apparatus. In some embodiments, the shell protects of the interior of the ultrasound imaging apparatus from ingress of fluids and dust.

In another broad aspect of the present disclosure, there is provided a method of detecting presence of a compatible cooling unit for attaching to an ultrasound imaging apparatus, the method including: providing a sensor on one of: the ultrasound imaging apparatus, and the cooling unit; providing an identity interface on the other of: the ultrasound imaging apparatus, and the cooling unit; when the cooling unit is attached, the identity interface is read through the sensor; and the attached cooling unit is detected to be compatible if the reading of the identity interface matches an expected reading.

In some embodiments, the method may be considered a method of determining whether a cooling unit is attached to an ultrasound imaging apparatus and/or whether or not it is compatible with said ultrasound imaging apparatus.

In some embodiments, the sensor is provided on the ultrasound imaging apparatus and the identity interface is provided on the cooling unit.

In some embodiments, the ultrasound imaging apparatus includes a first electrical connector capable of supplying current and the cooling unit includes a second electrical connector that interfaces with the first electrical connector. When the cooling unit is attached and determined to be compatible, the ultrasound imaging apparatus activates the first electrical connector to supply electric current to the second connector so that the cooling unit is powered.

In some embodiments, the first electrical connector is prevented from supplying current if the cooling unit is determined to be not compatible. In some embodiments, the ultrasound imaging apparatus is prevented from imaging if the cooling unit is determined to be not compatible.

In some embodiments, the sensor is provided on the cooling unit and the identity interface is provided on the ultrasound imaging apparatus. In some embodiments, the cooling unit is prevented from activating if the cooling unit is determined to be not compatible with the ultrasound imaging apparatus.

In another broad aspect of the present disclosure, there is provided a cooling unit for an ultrasound imaging apparatus, the cooling unit including: a housing, the housing including a fastener for detachably coupling to the ultrasound imaging apparatus; and an active cooling element, wherein the active cooling element is enclosed in the housing, and the active cooling element is configured to remove heat from the ultrasound imaging apparatus; wherein the cooling unit is cordless.

4

In some embodiments, the active cooling element includes a fan configured to direct air onto or away from an external surface of the ultrasound imaging apparatus.

In some embodiments, the cooling unit housing includes at least one air inlet and at least one air outlet. In some embodiments, a size of the air inlet is different (e.g., larger) from the size of the air outlet to induce a pressure differential.

In some embodiments, the cooling unit includes an electrical connector for receiving power from the ultrasound imaging apparatus to power the active cooling element.

In some embodiments, the cooling unit includes an internal battery for providing power to the active cooling element.

In some embodiments, the fastener is formed with the housing, and the housing includes at least one clip for performing the detachable coupling.

In some embodiments, the housing includes at least one magnet for performing the detachable coupling and the ultrasound imaging apparatus includes a portion of the body for mating with the at least one magnet.

In some embodiments, the cooling unit is waterproof allowing for, for example, cleaning with liquids.

In some embodiments, the cooling unit is dustproof allowing for operation in environments with small particles which may negatively affect the performance of the cooling unit.

For simplicity and clarity of illustration, where considered appropriate, reference numerals may be repeated among the figures to indicate corresponding or analogous elements or steps. In addition, numerous specific details are set forth in order to provide a thorough understanding of the exemplary embodiments described herein. However, it will be understood by those of ordinary skill in the art that the embodiments described herein may be practiced without these specific details. In other instances, certain steps, signals, protocols, software, hardware, networking infrastructure, circuits, structures, techniques, well-known methods, procedures and components have not been described or shown in detail in order not to obscure the embodiments generally described herein.

Furthermore, this description is not to be considered as limiting the scope of the embodiments described herein in any way. It should be understood that the detailed description, while indicating specific embodiments, are given by way of illustration only, since various changes and modifications within the scope of the disclosure will become apparent to those skilled in the art from this detailed description. Accordingly, the specification and drawings are to be regarded in an illustrative, rather than a restrictive, sense.

Referring to FIG. 1, shown there generally as **100** is a schematic representation of an ultrasound imaging system, in accordance with at least one embodiment of the present invention. As shown, the ultrasound imaging system includes an ultrasound imaging apparatus **110** and an active cooling unit **130** that can detachably couple to the ultrasound imaging apparatus **110**.

The ultrasound imaging apparatus **110** may contain a transducer **114** which may be configured to emit ultrasound energy signals towards an object and receive echoes of the ultrasound energy signals that reflect off the object. Transducer **114** may be electrically connected to electronics **116** which can control the transducer **114** and process the received echoes into ultrasound image data. Ultrasound imaging apparatus **110** may have a battery **118** for providing power to the electronics **116**. Ultrasound imaging apparatus **110** may have a heat dissipater **120** that receives heat from

5

the electronics **116** and/or transducer **114** and/or battery **118** during operation. Active cooling unit **130** may include a fastener **136** for facilitating the detachable physical coupling of the active cooling unit **130** to the ultrasound imaging apparatus **110**. When it is attached, active cooling unit **130** can be configured to remove heat from the ultrasound imaging apparatus' heat dissipater **120** using active cooling element **140**. Active cooling unit **130** may include a connector **132** that electrically connects to the corresponding connector **122** on the ultrasound imaging apparatus **110** when the active cooling unit **130** is coupled to ultrasound imaging apparatus **110**. In various embodiments, connector **132** may serve different purposes. For example, the electrical connection between connector **132** and connector **122** may enable ultrasound imaging apparatus **110** to provide power to active cooling element **140**, and/or enable ultrasound imaging apparatus **110** to determine when a compatible active cooling unit **130** is attached.

During operation, ultrasound imaging apparatus **110** may transmit ultrasound image or other data to a tertiary device for display or storage. For example, ultrasound imaging apparatus **110** may transmit data via a wired or wireless connection to a multi-use electronic display device to display an ultrasound image.

In various embodiments, the cooling unit **130** may generally be provided in a cordless form that can operate without attached wires or cords (e.g., either for supplying power or for transferring heat away from the cooling unit **130**). Corded devices may generally be cumbersome to use, and the cooling unit **130** being cordless may provide enhanced ease of use.

Referring to FIG. 2A and FIG. 2B, shown there generally as **200A** and **200B**, respectively, are perspective views of an example embodiment of an ultrasound imaging system, in accordance with at least one example embodiment of the present invention. FIG. 2A shows ultrasound imaging system **200A** with ultrasound imaging apparatus **110** and active cooling unit **130** in a detached state. FIG. 2B shows the same ultrasound imaging system **200B**, with ultrasound imaging apparatus **110** and active cooling unit **130** in an attached state.

The ultrasound imaging apparatus **110** generally has a shell **211** which may be connected to a transducer array **114** and, internal to the shell, the processing components. As the ultrasound imaging apparatus **110** is used to perform imaging, heat may be generated by the transducer array **114** and/or the processing components (e.g., the electronics **116** shown in FIG. 1) and/or the battery **118**. As shown in FIG. 2A, a heat dissipater **120** shown in FIG. 1 is provided as fins **220** on the shell **211** of the ultrasound imaging apparatus **110**. The fins **220** help to passively dissipate heat from the ultrasound imaging apparatus **110** using natural convection. While fins **220** may generally provide a sufficient level of heat dissipation, it may be desirable to further enhance the heat dissipation in certain circumstances. For example, further enhancing the heat dissipation may allow for continuous scanning by the ultrasound imaging apparatus **110** over a lengthy period.

To increase the heat dissipated from ultrasound imaging apparatus **110**, active cooling unit **130** may be attached (as shown in FIG. 2B). Active cooling unit **130** generally has a main body **231**, and may also include a fastener for detachably coupling the active cooling unit **130** to the ultrasound imaging apparatus **110**. In the example embodiment of FIGS. 2A-2B, the fastener is formed with the main body **231** as a clip portion **236** that facilitates attachment of the cooling unit **130** to the ultrasound imaging apparatus **110**. The main

6

body **231** may also include air inlets **242** and air outlets **244** to allow air to flow past and/or through the active cooling element (not shown in FIGS. 2A and 2B).

In this illustrated embodiment, cooling unit **130** attaches to ultrasound imaging apparatus **110** using a fastener provided in the form of clip portion **236**. Clip portion **236** can be made of a suitably flexible material to allow the clip portion **236** to flex around/over the shell **211** and snap on/off of the ultrasound imaging apparatus **110**. In various embodiments, the material of clip portion **236** and/or the main body **231** of the cooling unit **130** may be selected to provide additional heat conduction from shell **211** to active cooling unit **130**. The coupling mechanism may be releasable without the use of tools, as is the case with the example flexible clip portion **236**. However, in some embodiments, the use of tools for releasing the cooling unit **130** may be possible.

In some embodiments, the coupling mechanism (e.g., the fastener) may be configured to maintain a specific relative position between the active cooling unit **130** and the ultrasound imaging apparatus **110**. This may facilitate improved heat transfer over embodiments without such relative positioning. For example, as illustrated, the clip portion **236** may be shaped to match the profile of a portion (e.g., shell **211**) of the ultrasound imaging apparatus **110**. The matching of the clip portion **236** to one or more of the profile, shape, and/or curvature of the shell **211** may allow the cooling unit **130** to be positioned substantially over the fins **220** so that the active cooling element can operate primarily thereon. This, in turn, may enhance the heat dissipated from the fins **220**.

Referring to FIG. 3, shown there generally as **230** is a rear perspective view of an active cooling unit **130**, in accordance with at least one embodiment of the present invention. As noted with respect to FIG. 1, the active cooling unit **130** may include an active cooling element **140**. In the example embodiment shown in FIG. 3, the active cooling element **140** is provided in the form of a fan **340** mounted to the main body **231**.

Connector **132** can also be mounted to main body **231**, and may form an electrical connection to the fan **340**. As discussed below, connector **132** may include several pins **334**, **335**, and **336** that can provide power to the fan and/or provide access to an identity interface when attached to the ultrasound imaging apparatus **110**. The at least one air inlet **242** and at least one air outlet **244** formed as holes in the housing **231** of the cooling unit **130** are also viewable in FIG. 3.

Referring to FIG. 4, shown there generally as **400** is a partial perspective view of the ultrasound imaging system of FIG. 2 with a broken-out section to show example airflow. During operation, cool air can be drawn into active cooling unit **130** through air inlets **242** along air inlet path **420** by fan **340**. Once through fan **340**, air can be directed into and along the fins **220** of the ultrasound imaging apparatus **110**. Heat can then be transferred from the fins **220** to the cool air through convection. The warm air may then continue to travel along air outlet path **430** through the air outlet **244** in housing **231** and into the surrounding environment. In this embodiment, the cool air can be directed onto the surface of the heat dissipater **120** (e.g., fins **220**) to generate more turbulence and enhance heat transfer. It can be appreciated that those skilled in the art may choose to use a different air pathway. For example, the fan may be configured to operate so that airflow is in the reverse direction so as to draw air away from an external surface of the ultrasound imaging apparatus **110**.

In some embodiments, the size and shape of air inlets 242 and air outlets 244 can be configured so that the air inlets 242 are different from the air outlets 244 (e.g., as shown, the air inlets 242 are larger than the air outlets 244). Such a configuration may create a pressure differential across the fan 340, so as to increase the pressure (and thus velocity) of the airflow downstream from the fan 340 directed at the fins 220. This, in turn, may improve heat dissipation performance. In various embodiments, the location of air inlets 242 and air outlets 244 may be chosen to direct the warm air away from the operator of the ultrasound imaging apparatus 110 and/or away from the patient during scanning.

Referring to FIG. 5, shown there generally as 500 is an electrical schematic for active cooling unit 130 of the ultrasound imaging system of FIGS. 2A-2B. The electrical schematic includes an ultrasound imaging apparatus portion 510 and an active cooling unit portion 530. The apparatus portion 510 and the active cooling unit portion 530 can be connected via pins 333, 334, 335 on the active cooling unit portion 530 and corresponding pins 523, 524, 525 on the apparatus portion 510. Each of the apparatus pins 523, 524, 525 may be connected to a processor 517 (e.g., microcontroller unit (MCU)). As discussed below, when the cooling unit portion 530 is attached to the apparatus portion 510, processor 517 may control the flow of electricity to the fan 340 and/or detect whether a cooling unit 130 encompassing the attached fan portion 530 circuit is compatible.

The electrical schematic of FIG. 5 may operate in a detached state and an attached state, and processor 517 can be configured to determine in which state the circuit is operating. In the detached state, pins 333, 334, and 335 are not electrically connected to target pins 523, 524, and 525, respectively. In the attached state, pins 333, 334, and 335 are electrically connected to target pins 523, 524, and 525, respectively.

Processor 517 may be configured to control power to fan 340 and therefore control when the fan 340 operates. Processor 517 may be connected to target pin 523 on apparatus portion 510, and fan 340 may be connected to pin 333 on cooling unit portion 530. In the attached state, pin 333 and target pin 523 are electrically connected. Processor 517 can then activate power to target pin 523 so that current flows through pin 333 to energize fan 340. In this mode of operation, pin 523 may be a live or hot pin that supplies current to the fan 340 through pin 333, and pin 525 may be the neutral pin that returns current to the processor 517 through pin 335 connected to fan 340. In the detached state, processor 517 may deactivate power to target pin 523 and prevent electric current from flowing thereto. In some embodiments, processor 517 activates the fan 340 whenever the active cooling unit 130 is determined to be attached.

A processor 517 may determine whether a compatible cooling unit 130 is attached in various ways. For example, as illustrated, the compatible cooling unit 130 may include the cooling unit portion 530 of the circuit shown in FIG. 5. Detector pin 524 may be provided on the apparatus portion 510 that, in the attached state, mates with a corresponding identity pin 334 on the cooling unit portion 530 to form an electrical connection. The electronics between detector pin 524 and neutral pin 525 connected within the apparatus portion 510 (e.g., including processor 517 and voltage source 550 (labeled as '+Vcc')) may be considered circuitry for detecting the presence of a cooling unit 130. In the illustrated embodiment, this detection circuitry includes a first portion of a voltage divider circuit, having resistor 519A (labeled as 'R2'), resistor 519B (labeled as 'R3'), and resistor 519C (labeled as 'R4').

In operation, the processor 517 may be configured to measure voltage in the detection circuitry at regular intervals to determine whether a compatible cooling unit portion 530 is attached. For example, in the detached state, there is typically no electrical connection between detector pin 524 and neutral pin 525 on the apparatus portion 510. This would result in significant resistance across those two pins, such that current is unlikely to flow through resistor 519B from the voltage source 550. As a result, current will generally flow from the voltage source 550 through resistor 519A towards resistor 519C so as to produce a first predetermined voltage measurement between the connection point 560 and connection point 565 (This first predetermined voltage measurement would depend on the resistance of the resistors 519A, 519C). If a measured voltage that is taken periodically matches this first predetermined voltage measurement, the processor 517 may determine that a compatible cooling unit 530 is not attached. For example, the processor 517 may then substantially limit the flow of current towards the pin 523 from voltage source 550.

As illustrated, active cooling unit portion 530 may include a second portion of a voltage divider circuit having resistor 545. When the active cooling portion 530 is attached, an electrical connection may be formed between detector pin 524 and neutral pin 525 on the apparatus portion 510 (e.g., through identity pin 334, resistor 545, and pin 335 on the cooling unit portion 530). This electrical connection may complete the voltage divider circuit, and draw current towards resistor 519B at the connection point between resistor 519A and resistor 519C. Current may then flow through resistor 545, and back towards connection point 565 at processor 517. Since some current has been divided away from the circuit having resistors 519A and 519C, a voltage measurement taken across connection points 560 and 565 will be different from the first predetermined voltage measurement when there was no cooling unit portion 530 attached and there was substantial resistance across target pins 524 and 525. The resistance of the resistor 545 on the cooling unit portion 530 may be selected so that when the cooling unit portion 530 is attached, a predetermined voltage at connection point 560 is experienced. In various embodiments, if the periodically measured voltage matches a second predetermined voltage across the connection point 560 and connection point 565 (e.g., the amount of voltage divided away from the first predetermined voltage measurement is consistent with that which is expected based on the expected resistance provided by resistor 545), then the processor 517 may determine that a compatible cooling unit 545 is attached.

However, if the electrical circuit between detection pin 524 and neutral pin 525 is complete, but the measured voltage does not match the second predetermined voltage (e.g., the amount of voltage divided away from the first determined voltage measurement above is inconsistent with an expected resistance of resistor 545 based on the design of a compatible cooling unit portion 530), the processor 517 may determine that an incompatible cooling unit 130 is attached. To facilitate ease of manufacturing and/or ease of sourcing of components, the second predetermined voltage may include different resistance values corresponding to different resistors, so that if the measured voltage matches any one of these different resistance values, the attached cooling unit portion 530 may be determined to be compatible.

In another scenario, it may be possible that target pin 524 and target pin 525 on the apparatus portion 510 are shorted such that there is little to no resistance experienced between

the two pins. For example, this may happen if the ultrasound imaging apparatus **110** is submerged in water or other conductive liquid during cleaning. This may result in another predetermined voltage experienced across: either voltage source **550** and connection point **560**, or between connection points **560** and **565**. If any voltage measurement matches such predetermined voltage, then the processor **517** may also determine that a compatible cooling unit **130** has not been attached, so as to also substantially limit the flow of current towards pin **523** from voltage source **550**.

In various embodiments, when determining whether a measured voltage matches a predetermined voltage, the processor **517** may not necessarily identify a precise voltage. Instead, if a measured voltage is within a known variance of the predetermined voltage (e.g., within an expected range based on component specifications), the measured voltage may still be considered as matching. For example, when selecting the lower and upper bounds of an expected voltage range, the next lower and next higher standard values of resistors may be taken into account. For an example target resistance of 2K ohms, the adjacent standard values in the IEC 60063 E96 series are 1.96K ohms and 2.05K ohms. Thus, these values may be selected to be the lower and upper bounds of an expected voltage range if the 2K ohm resistor is selected as resistor **545** to be placed into a compatible cooling unit **130**.

In the manner discussed, the resistance of resistor **545** may serve as an identity interface that allows the apparatus portion **510** to determine whether an attached cooling unit portion **530** is compatible. For example, the reading of the identity interface by the apparatus portion **510** may facilitate detection of counterfeit and/or malfunctioning cooling units **130**. Since such non-compatible cooling units **130** may not be configured to safely handle the electrical current supplied via live pin **523** when pin **523** is activated, the processor **517** may be configured to only activate current flow to pin **523** if an attached cooling unit **130** is determined to be compatible. This may provide enhanced safety and reduce the possibility of electric shock. As discussed below, this may also allow the pins **523**, **524**, **525** to be exposed to liquids such as water when cleaning the ultrasound imaging apparatus.

As discussed above, the processor may use the identify interface on the cooling unit portion **530** to determine when to supply power to pin **523** for activating the fan **340**. However, in some embodiments, processor **517** may use additional or alternative information to determine when to supply power to pin **523**. For example, the processor **517** may activate or deactivate current flow to pin **523** based on a current imaging mode of the ultrasound imaging apparatus **110**; a temperature measured within the ultrasound imaging apparatus **110**; and/or based on input from the operator.

In some embodiments, the circuit may include protective circuitry. For example, as shown in the example circuit of FIG. 5, a snubber diode **543** is connected in reverse parallel with fan **340** to prevent inductive kickback. As shown in FIG. 5, a diode **521** is also connected to detector pin **524** to prevent current flow towards connection point **560** in a manner that may potentially result in an erroneous determination that a compatible cooling unit **130** has been attached. Various other embodiments may also include components to prevent damage to the ultrasound imaging apparatus **110** from electrostatic discharge or unexpected connections.

As discussed herein, the detection circuitry provided on the apparatus portion **510** may be considered a sensor that reads the identity interface provided on the cooling unit **130**. In various embodiments, other types of sensors may be used

to determine whether a compatible active cooling unit **130** is attached to the ultrasound imaging apparatus **110**. For example, the sensor may include a mechanical switch, a magnet and reed switch, and/or a radio frequency identification (RFID) tag. Other known or later developed sensors capable of detecting the attachment of the active cooling unit can be used.

Referring to FIG. 6, shown there generally as **600** is a flow chart depicting a method for determining whether an attached active cooling unit is compatible with an ultrasound imaging apparatus, according to at least one embodiment of the present invention. The method may be performed by the ultrasound imaging apparatus **110**. Alternatively, the method may be performed by the active cooling unit **130**.

At **610**, a sensor may be provided on an ultrasound imaging apparatus **110** or an active cooling unit **130**. The sensor may be any suitable component or combination of components that allows for reading an identity interface. For example, as noted, the portion of the detection circuit like that which is provided on the apparatus portion **510** (e.g., including a portion of a voltage divider circuit and processor **517**) may be considered a sensor.

At **620**, an identity interface may be provided on the other of the active cooling unit **130** and the ultrasound imaging apparatus **110**. The identity interface may be any component (or combination of components) that allows a corresponding sensor to determine whether a cooling unit **130** is compatible. For example, in the detection circuitry of FIG. 5, the identity interface includes a resistor **545** with a predetermined resistance that completes the voltage divider circuit in the sensor when the cooling unit **130** having the cooling unit portion **530** is attached to the apparatus portion **510**.

At **630**, the sensor may read the identity interface when the active cooling unit **130** is attached to the ultrasound imaging apparatus **110**. The reading of the identity interface may be performed in various ways. For example, in the example embodiment of FIG. 5 where the sensor is a portion of a voltage divider circuit, the reading may be performed by a processor **517** taking periodic voltage measurements as discussed above. When the cooling unit **130** is attached, a voltage at connection point **560** can be read and compared with a predetermined value.

At **640**, the compatibility of the active cooling unit **130** is determined. Compatibility may be determined in various ways. For example, determining compatibility may involve comparing a value read at act **630** with one or more predetermined values. As discussed above, in example embodiment where the identity interface includes a resistor **545**, these predetermined values may be an expected range of resistance values for resistors that have been selected for inclusion in compatible cooling units **130**. In the manner discussed, the identity interface may serve to “identify” the cooling unit **130** to the imaging apparatus **110**. This may help ensure any attached cooling unit **130** used with the imaging apparatus **110** is not counterfeit and/or has met sufficient quality and safety standards.

If the active cooling unit **130** is determined to be incompatible, one or more different actions may be taken. For example, the operator may be alerted. Additionally or alternatively, if the active cooling unit **130** would normally receive power from the ultrasound imaging apparatus **110** through an electrical connection, the power may be disabled. Additionally or alternatively, the ultrasound imaging apparatus **110** may be prevented from imaging.

If the active cooling unit is determined to be compatible, one or more other actions may be taken. For example, as noted, the ultrasound imaging apparatus **110** may provide

11

electrical power through an electrical connection to power and activate the active cooling unit **130**. If the active cooling unit **130** is independently powered, the ultrasound imaging apparatus may instruct the active cooling unit **130** to begin cooling.

While the illustrated embodiment provides an identity interface in the form of a resistor **545** being part of a voltage divider circuit (with the corresponding sensor being the remaining portion of the voltage divider circuit), different embodiments may provide an identity interface and corresponding sensor in various ways. For example, any combination of electrical, mechanical, digital, optical, wireless, or software-based components can be provided as an identity interface, and a suitable sensor may be used for identifying the identity interface and determining compatibility. Also, as illustrated herein, the sensor is provided on the ultrasound imaging apparatus **110** and the identity interface is provided on the cooling unit **130**. However, in various embodiments, the positioning of these elements may be reversed: e.g., the sensor may be provided on the cooling unit **130**, and the identity interface may be provided on the imaging apparatus **110**.

Although the cooling units discussed herein have generally referred to active cooling units, the methods of FIG. **6** may also be performed on passive cooling units in various embodiments. A passive cooling unit may dissipate heat without the need for electrical energy. For example, cooling unit **130** may include a heat sink thermally connected to a heat transfer surface. The heat transfer surface may be configured to thermally mate with the heat dissipating portion **120** of the imaging apparatus **110**, so that heat from the imaging apparatus **110** is transferred to the heat sink and dissipated. In another example, cooling unit **130** may include a heat storage device to temporarily store heat from the imaging apparatus **110**. As discussed herein, detecting the compatibility of a passive cooling unit may allow the ultrasound imaging apparatus to modify its operation (e.g., allow/disallow imaging, and/or modifying imaging parameters).

Referring to FIG. **7A**, shown there generally as **700A** is a front view of the ultrasound imaging system of FIGS. **2A-2B**. The connector **122** on ultrasound imaging apparatus **110** may have target pins **523, 524, 525** (as discussed above in relation to FIG. **5**). In various embodiments, these target pins **523, 524, 525** may be provided in the form of exposed electrical pads that can be powered when a cooling unit **130** is attached. Having such exposed electrical connection points may potentially result in risk of electric shock if the pins become powered unexpectedly. As noted above, configuring the pins to detect that a cooling unit **130** is compatible prior to powering the pins may enhance safety and reduce the risk of electric shock.

Additionally, having exposed electrical connection points may traditionally make it more difficult to clean or sterilize the ultrasound imaging apparatus **110**. This is because having exposed electrical connections may require openings to be provided on the external shell **211**. In turn, these openings may potentially allow a cleaning agent (e.g., water or other disinfectant liquid) to ingress into the interior of the ultrasound imaging apparatus **110** to damage the electronics contained therein. Notwithstanding these challenges, in some embodiments of the present invention, the construction of the exposed electrical connections through shell **211** may protect from ingress of fluid and dust into the interior of ultrasound imaging apparatus **110**. For example, in various embodiments, the shell **211** may satisfy an International Electrotechnical Commission (IEC) rating of at least IPX7.

12

Referring to FIG. **7B**, shown there generally as **700B** is an enlarged partial perspective view of the connector **122** of the ultrasound imaging apparatus **110** of FIGS. **2A-2B**. As shown in FIG. **7B**, the openings **780** in the shell **211** providing access to the electrical pads **523, 524, 525** of connector **122** may be sealed from the interior of the ultrasound imaging apparatus **110** via waterproof tape **752**. In an example embodiment, one or more hole(s) may be cut in the waterproof tape **752** so that the hole(s) expose corresponding electrical pads **523, 524, 525**. One side of the tape may be adhered to a printed circuit board (PCB) having the electrical pads **523, 524, 525** that can mate to pins **333, 334, 335** of the active cooling unit **130**; and the other side of the tape **752** may be adhered to the interior surface of the shell **211** (either directly or indirectly through another medium that provides sealing and still exposes the electrical pads). This may allow the electrical pads **523, 524, 525** to be exposed through the waterproof tape **752** and the shell **211** while maintaining ingress protection of liquids and other materials into the interior of the ultrasound imaging apparatus **110**.

Referring to FIG. **7C**, shown there generally as **700C** is a cross-sectional view of the ultrasound imaging system of FIG. **2A-2B** along line C-C show in FIG. **7A**, in accordance with at least one embodiment of the present invention. In the cross-sectional view of FIG. **7C**, the cooling unit **130** is attached to the ultrasound imaging apparatus **110**, with the clip portion of the cooling unit **130**'s main body **231** fitting around the outer shell **211** of the ultrasound imaging apparatus **110**.

Referring to FIG. **7D**, shown there generally as **700D** is a detail view of the area highlighted by 'D' in FIG. **7C**, in accordance with at least one embodiment of the present invention. In this view, the waterproof tape **752** is viewable. The lower side of the waterproof tape **752** is adhered to the PCB **754** having the electrical pads **523, 524, 525** and the upper side of the waterproof tape **752** is adhered to the interior of the interior surface of the shell **211**. The pins **333, 334, 335** may penetrate the holes in the waterproof tape **752** to mate with the exposed electrical pads **523, 524, 525**, and form an electrical connection therewith. In various embodiments, one or more pins **333, 334, 335** may be provided as spring-loaded pins. For example, this may allow for a solid electrical connection by providing secure contact between the pin and the exposed electrical pads. For example, one option for spring-loaded pins is POGO™ pins from Everett Charles Technologies. In various embodiments, the spring-loaded pins and the target exposed pads should be chosen of a material that is suitable for immersion in a cleaning or disinfection solution.

Various embodiments discussed herein may configure the ultrasound imaging apparatus **110** to be protected from ingress. As discussed, this may facilitate ease of cleaning (e.g., allow for wiping with disinfection solution and/or allow for the ultrasound imaging apparatus **110** to be submerged in liquid). The embodiments may be configured to maintain this ingress protection even with exposed electrical connectors that mate with electrical connectors from the cooling unit **130**.

In the example embodiment shown in FIG. **7A-7C**, waterproof tape **752** is discussed as providing the sealing mechanism that provides ingress protection. However, it will be understood that other suitable methods (e.g., other types of mechanical fasteners, sealants, gaskets, O-rings) for providing ingress protection while still providing exposed electrical connectors may be possible.

13

Referring to FIG. 8, shown there generally as **800** is a perspective view of an embodiment of the present invention, with an alternative means of coupling the active cooling unit to the ultrasound imaging apparatus. Ultrasound imaging system **800** may include an ultrasound imaging apparatus **810** and a detachable active cooling unit **830**. Active cooling unit **830** may have a housing **831** configured with at least one magnet **836**. The at least one magnet **836** may couple to shell **811**, and thereby allow fastening of the detachable active cooling unit **830** to the ultrasound imaging apparatus **810**. In various embodiments, different arrangements of magnets could be used. For example, permanent magnets could be attached onto both the cooling unit housing **831** and ultrasound imaging apparatus shell **811**. Alternatively, permanent magnets could be attached to one of the cooling unit **830** or the ultrasound imaging apparatus **810**; with the other component being formed with a magnetically responsive material, so as to allow a magnetic connection to be formed therebetween (e.g., mating between the cooling unit **830** and the ultrasound imaging apparatus **810**). In some embodiments, the orientation of the magnets coupled with different polarities provide the ability to align the cooling unit **830** to the ultrasound imaging apparatus **810**.

Referring to FIG. 9, shown there generally as **900** is a perspective view of another alternative embodiment of the present invention, where the active cooling unit is powered independently. Ultrasound imaging system **900** may include an ultrasound imaging apparatus **910** and a detachable active cooling unit **930**. Like the example cooling units **130** discussed above, the active cooling unit **930** may have a body portion **931** that is formed with a clip portion **936** for securing around the shell **911** of the ultrasound imaging apparatus **910**.

However, unlike the ultrasound imaging apparatus **110** discussed above, the ultrasound imaging apparatus **910** may be configured to not have a connector **122** for supplying power to the cooling unit **930**. For example, this may simplify design or manufacturing of the ultrasound imaging apparatus **910**. Additionally or alternatively, this may allow cooling units **930** to be interoperable with configurations of the ultrasound imaging apparatus without connector **122**. Since the imaging apparatus may be configured without connector **122**, the cooling unit **930** may similarly be configured to not have a corresponding connector **132** (as shown earlier in FIG. 3).

Instead, in the embodiment of FIG. 9, the active cooling unit **930** may include an internal power source such as a battery. The battery may provide power to the active cooling element **140** (as shown in FIG. 1) to help remove heat from ultrasound imaging apparatus **910**. In various embodiments, the internal battery may be rechargeable or single-use. In various embodiments, the internal battery may be removable or non-removable. In various embodiments, the cooling unit **930** may be provided with a switch that allows for the activation and/or deactivation of the active cooling element.

Referring to FIG. 10, shown there generally as **1000** is a perspective view of another alternative embodiment of the present invention, with both the magnetic coupling mechanism discussed above in relation to FIG. 8 and an internally powered active cooling element discussed above in relation to FIG. 9. An ultrasound imaging system **1000** may include an ultrasound imaging apparatus **1010** and a detachable active cooling unit **1030**. The active cooling unit **1030** may include a housing **1031** which has at least one magnetic fastener **1036**. Various configurations of coupling can be used as described in FIG. 8 above. The active cooling unit **1030** may also be self-powered, in a manner like how the

14

active cooling unit **930** discussed above was internally powered. Accordingly, the ultrasound imaging apparatus **1010** and the active cooling unit **1030** may not be provided with respective connectors **122/132** (as shown in FIG. 1)

Referring to FIG. 11, shown there generally as **1100** is a perspective view of another alternative embodiment of the present invention that has a different configuration of a heat dissipater. In various embodiments discussed above, the cooling unit **130** has been shown as being coupled to ultrasound imaging apparatus with finned heat dissipaters **220** (as shown in FIG. 2A). However, such fins **220** may not be present in various embodiments. For example, as shown in FIG. 11, the heat dissipating portion **1120** of ultrasound imaging apparatus **1110** may be a surface that is substantially smooth (e.g., without fins). Even without fins, the operation of the active cooling unit **1130** to project air towards and/or away from the relatively smooth surface **1120** may still provide a cooling effect on the ultrasound imaging apparatus **1110**.

The embodiment illustrated in FIG. 11 is shown as having a housing **1131** that incorporates a clip portion **1136**. Also, the ultrasound imaging apparatus **1110** in FIG. 11 is shown as having a connector portion **1122**. However, the various potential modifications discussed herein (e.g., magnetic coupling, self-powered without connectors **1122**) may also be made to the embodiment of FIG. 11.

Referring again to FIGS. 3, 5, and 6, the example illustrated embodiments are shown as having three (3) pins **333**, **334**, **335** on the connector **132** of the cooling unit **130**, with three (3) corresponding target pins provided on the ultrasound imaging apparatus **110**. In various embodiments, there are a different number of pins provided on the connectors **122**, **132** connecting the active cooling unit **130** to the ultrasound imaging apparatus **110**. For example, in some embodiments, there may be only two (2) pins provided on the connectors **122**, **132**. This may be the case if the only two pins are provided (e.g., when activated, a live pin and a neutral pin), but the detector pin **524** (as shown in FIG. 5) is not provided. In these embodiments, the activation/deactivation of the active cooling element may be based on a suitable switch that is not contingent on the identification of a compatible cooling unit **130**.

In other embodiments, there may be only a single pin provided on the connectors **122**, **132** connecting the active cooling unit **130** to the ultrasound imaging apparatus **110**. For example, this may be the case if the active cooling unit **130** is self-powered, and only the detector pin **524** and corresponding identity interface pin is provided to determine if an attached cooling unit **130** is compatible. In these embodiments, the ultrasound imaging apparatus **110** may be configured to not allow imaging to proceed if a non-compatible cooling unit **130** is determined to be attached.

In some embodiments, active cooling unit **130** may receive power from ultrasound imaging apparatus **110** without the use of a conductor-based (e.g., wired) electrical connection. For example, various conventionally known or future-developed wireless power transfer techniques may be used provide power to active cooling unit **130**. For example, inductive coupling, capacitive coupling, and/or magnetodynamic coupling may be used to transfer power from ultrasound imaging apparatus **110** to active cooling unit **130** to power active cooling element **140**.

Although the active cooling element **140** has generally been described herein as being provided in the form of fan **340**, other types of active cooling element are possible. Various conventionally known or future developed active cooling elements may be used to remove heat from the

ultrasound imaging apparatus **110**. For example, a thermo-electric cooler or a refrigeration cycle-based heat pump may be used alone or in combination to provide active cooling.

As illustrated herein, the ultrasound imaging apparatus **110** is shown as being in the form of a wireless ultrasound scanner that may connect via wireless communication protocols to a suitable display for displaying the ultrasound image data generated from the scanner. However, the present embodiments can be practiced with ultrasound imaging apparatus of any types, whether wired or wireless. By providing a cooling unit **130** that either draws power from the ultrasound imaging apparatus **110** or is self-powered (as discussed above), the cooling unit **130** can provide the advantages of active cooling while still being cordless. This may facilitate ease of attachment and portability for the cooling unit **130** for either wired or wireless ultrasound imaging apparatus **110**. This may also allow for scanning of longer duration for ultrasound imaging apparatus **110** that is either wired or wireless.

In various embodiments, the ultrasound imaging apparatus **110** may be configured to control activation of a cooling unit **130** based on temperature sensors provided within the ultrasound imaging apparatus **110**. For example, an ultrasound operator may wish to perform an ultrasound examination in a location with a high ambient temperature. The ultrasound operator may attach the active cooling unit **130** to the ultrasound imaging apparatus **110** and begin scanning. When the active cooling unit **130** is attached, an electrical connection may be formed, which may allow a processor within the ultrasound imaging apparatus **110** to detect the cooling unit's **130** presence and control power to it. The ultrasound imaging apparatus **110** may be provided with temperature sensor(s) that the processor may monitor. If the temperature exceeds a predetermined value, the processor may turn on the active cooling unit **130**. When powered on, the active cooling element (e.g., a fan) may force air past a heat dissipating portion of the ultrasound imaging apparatus **110**, and enhance the cooling beyond natural convection. This may allow the ultrasound operator to continue scanning in a situation where the temperature sensor may otherwise need to stop the ultrasound imaging apparatus **110** from scanning due to high temperatures.

In various embodiments, the ultrasound imaging apparatus **110** may adjust imaging parameters based on the status of attachment of cooling unit **130**. Since an attached cooling unit **130** may allow the ultrasound imaging apparatus **110** to operate with a higher processing load that generates more heat, these adjustments may increase image quality or imaging performance when the cooling unit **130** is attached. Correspondingly, the ultrasound imaging apparatus **110** may decrease image quality or imaging performance when the cooling unit **130** is detached (e.g., to lower processing load and thus, heat generation). For example, a frame acquisition rate, a line density, or other imaging parameter may be increased to provide better image quality when the cooling unit **130** is attached.

In various embodiments, the identity interface may provide additional information to the imaging apparatus **110**. For example, the identity interface may be configured to provide information about the heat dissipating capacity of the cooling unit **130**. The heat dissipation information may be used by the imaging apparatus **110** to change imaging parameters to achieve a desired run time. In another example, the heat dissipating capacity information may be used by the imaging apparatus **110** to provide an estimated run time to the user.

In various embodiments, the active cooling unit **130** may be provided in different configurations or forms having varying types of active cooling elements **140**. For example, these different configurations may be recognized and/or differentiated by the ultrasound imaging apparatus **110** using the identity interface. In example embodiment, one configuration of the active cooling unit **130** may have a small, lightweight fan configured to remove a relatively small amount of heat (while consuming relatively small amount of power); and a second configuration of the cooling unit **130** may have a larger, heavier (and potentially bulkier) fan capable of removing more heat but drawing more power. The ultrasound imaging apparatus **110** may distinguish between the two active cooling units and provide different estimates of allowable run-time, and/or activate different imaging modes as described above.

In some cases, the ultrasound imaging apparatus **110** may continue to increase in temperature even after the cooling unit **130** is running. If a second predetermined temperature threshold is detected, the ultrasound imaging apparatus **110** may be configured to alert the ultrasound operator (e.g., via a light-emitting diode (LED), audio, or through a suitable display device) that the ultrasound imaging apparatus **110** may stop scanning. In various embodiments, the active cooling unit **130** may continue running after scanning has been stopped to cool the ultrasound imaging apparatus **110**. The ultrasound operator may be alerted when the imaging apparatus is cool enough to resume scanning.

When the ultrasound operator wishes to perform an exam that is relatively short in duration, they may simply remove the detachable cooling unit **130** and scan normally.

While a number of exemplary aspects and embodiments have been discussed above, those of skill in the art will recognize that may be certain modifications, permutations, additions and sub-combinations thereof. While the above description contains many details of example embodiments, these should not be construed as essential limitations on the scope of any embodiment. Many other ramifications and variations are possible within the teachings of the various embodiments.

Interpretation of Terms

Unless the context clearly requires otherwise, throughout the description and the claims:

“comprise”, “comprising”, and the like are to be construed in an inclusive sense, as opposed to an exclusive or exhaustive sense; that is to say, in the sense of “including, but not limited to”;

“connected”, “coupled”, or any variant thereof, means any connection or coupling, either direct or indirect, between two or more elements; the coupling or connection between the elements can be physical, logical, or a combination thereof;

“herein”, “above”, “below”, and words of similar import, when used to describe this specification, shall refer to this specification as a whole, and not to any particular portions of this specification;

“or”, in reference to a list of two or more items, covers all of the following interpretations of the word: any of the items in the list, all of the items in the list, and any combination of the items in the list;

the singular forms “a”, “an”, and “the” also include the meaning of any appropriate plural forms.

Unless the context clearly requires otherwise, throughout the description and the claims:

Words that indicate directions such as “vertical”, “transverse”, “horizontal”, “upward”, “downward”, “forward”, “backward”, “inward”, “outward”, “vertical”, “transverse”,

“left”, “right”, “front”, “back”, “top”, “bottom”, “below”, “above”, “under”, and the like, used in this description and any accompanying claims (where present), depend on the specific orientation of the apparatus described and illustrated. The subject matter described herein may assume various alternative orientations. Accordingly, these directional terms are not strictly defined and should not be interpreted narrowly.

Embodiments of the invention may be implemented using specifically designed hardware, configurable hardware, programmable data processors configured by the provision of software (which may optionally comprise “firmware”) capable of executing on the data processors, special purpose computers or data processors that are specifically programmed, configured, or constructed to perform one or more steps in a method as explained in detail herein and/or combinations of two or more of these. Examples of specifically designed hardware are: logic circuits, application-specific integrated circuits (“ASICs”), large scale integrated circuits (“LSIs”), very large scale integrated circuits (“VLSIs”), and the like. Examples of configurable hardware are: one or more programmable logic devices such as programmable array logic (“PALs”), programmable logic arrays (“PLAs”), and field programmable gate arrays (“FPGAs”). Examples of programmable data processors are: microprocessors, digital signal processors (“DSPs”), embedded processors, graphics processors, math co-processors, general purpose computers, server computers, cloud computers, mainframe computers, computer workstations, and the like. For example, one or more data processors in a control circuit for a device may implement methods as described herein by executing software instructions in a program memory accessible to the processors.

For example, while processes or blocks are presented in a given order herein, alternative examples may perform routines having steps, or employ systems having blocks, in a different order, and some processes or blocks may be deleted, moved, added, subdivided, combined, and/or modified to provide alternative or subcombinations. Each of these processes or blocks may be implemented in a variety of different ways. Also, while processes or blocks are at times shown as being performed in series, these processes or blocks may instead be performed in parallel, or may be performed at different times.

The invention may also be provided in the form of a program product. The program product may comprise any non-transitory medium which carries a set of computer-readable instructions which, when executed by a data processor (e.g., in a controller and/or ultrasound processor in an ultrasound machine), cause the data processor to execute a method of the invention. Program products according to the invention may be in any of a wide variety of forms. The program product may comprise, for example, non-transitory media such as magnetic data storage media including floppy diskettes, hard disk drives, optical data storage media including CD ROMs, DVDs, electronic data storage media including ROMs, flash RAM, EPROMs, hardwired or pre-programmed chips (e.g., EEPROM semiconductor chips), nanotechnology memory, or the like. The computer-readable signals on the program product may optionally be compressed or encrypted.

Where a component (e.g. a software module, processor, assembly, device, circuit, etc.) is referred to above, unless otherwise indicated, reference to that component (including a reference to a “means”) should be interpreted as including as equivalents of that component any component which performs the function of the described component (i.e., that

is functionally equivalent), including components which are not structurally equivalent to the disclosed structure which performs the function in the illustrated exemplary embodiments of the invention.

Specific examples of systems, methods and apparatus have been described herein for purposes of illustration. These are only examples. The technology provided herein can be applied to systems other than the example systems described above. Many alterations, modifications, additions, omissions, and permutations are possible within the practice of this invention. This invention includes variations on described embodiments that would be apparent to the skilled addressee, including variations obtained by: replacing features, elements and/or acts with equivalent features, elements and/or acts; mixing and matching of features, elements and/or acts from different embodiments; combining features, elements and/or acts from embodiments as described herein with features, elements and/or acts of other technology; and/or omitting combining features, elements and/or acts from described embodiments.

It is therefore intended that the following appended claims and claims hereafter introduced are interpreted to include all such modifications, permutations, additions, omissions, and sub-combinations as may reasonably be inferred. The scope of the claims should not be limited by the preferred embodiments set forth in the examples, but should be given the broadest interpretation consistent with the description as a whole.

What is claimed is:

1. An ultrasound imaging system comprising:
 - a. an ultrasound imaging scanner operable to acquire ultrasound image data, the ultrasound imaging scanner comprising first electrical connection points on a handheld portion of the ultrasound imaging scanner; and
 - b. a cordless cooling unit configured to detachably couple to the handheld portion of the ultrasound imaging scanner, the cordless cooling unit comprising second electrical connection points, wherein when the cordless cooling unit is coupled to the handheld portion of the ultrasound imaging scanner, the second electrical connection points directly contact the first electrical connection points to form an electrical connection between the first electrical connection points on the handheld portion of the ultrasound imaging scanner and the second electrical connection points on the cordless cooling unit;
 - wherein the cordless cooling unit comprises an active cooling element to remove heat from the ultrasound imaging scanner, and when the cordless cooling unit is coupled to the handheld portion of the ultrasound imaging scanner, electricity for powering the active cooling element is supplied through the electrical connection formed between the first electrical connection points on the handheld portion of the ultrasound imaging scanner and the second electrical connection points on the cordless cooling unit.
2. The ultrasound imaging system of claim 1, wherein the ultrasound imaging scanner further comprises at least one sensor to detect when the cordless cooling unit is coupled.
3. The ultrasound imaging system of claim 2, wherein the at least one sensor comprises at least a portion of a resistor voltage divider network.
4. The ultrasound imaging system of claim 1, wherein the ultrasound imaging scanner comprises an external surface and the active cooling element comprises a fan, and wherein said fan is configured to direct air onto or from said external surface.

5. The ultrasound imaging system of claim 1, wherein the cordless cooling unit comprises at least one fastener to perform the detachable coupling.

6. The ultrasound imaging system of claim 1, wherein the ultrasound imaging scanner comprises a shell and wherein said shell protects from ingress into an interior of the ultrasound imaging scanner. 5

7. The ultrasound imaging system of claim 1, wherein the cooling unit further comprises an internal battery for powering the active cooling element. 10

8. The ultrasound imaging system of claim 1, wherein the fastener is formed with a housing of the cordless cooling unit, and the housing comprises at least one clip for performing the detachable coupling.

9. The ultrasound imaging system of claim 2, wherein an identity interface is provided on the cordless cooling unit, and the identity interface is read through the at least one sensor to detect when the cordless cooling unit is coupled. 15

10. The ultrasound imaging system of claim 9, wherein the ultrasound imaging scanner is configured to determine whether the coupled cordless cooling unit is compatible based on whether a reading of the identity interface matches an expected reading; and the ultrasound imaging scanner is further configured to limit or stop the electricity for powering the active cooling element supplied through the electrical connection when the cordless cooling unit is detected to be not compatible. 20 25

* * * * *