

US011331150B2

(12) **United States Patent**
Jascob et al.

(10) **Patent No.:** **US 11,331,150 B2**
(45) **Date of Patent:** **May 17, 2022**

(54) **METHOD AND APPARATUS FOR SURGICAL NAVIGATION**

(71) Applicant: **Medtronic Navigation, Inc.**, Louisville, CO (US)

(72) Inventors: **Bradley A. Jascob**, Broomfield, CO (US); **Laurent Verard**, Andover, MA (US); **Joel S. Hughes**, Erie, CO (US); **Steven L. Hartmann**, Superior, CO (US); **John J. Kappus**, Denver, CO (US); **Joseph Moctezuma**, Golden, CO (US); **Matthew F. Dicorleto**, Boulder, CO (US); **John B. Clayton**, Superior, CO (US)

(73) Assignee: **Medtronic Navigation, Inc.**, Louisville, CO (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1364 days.

(21) Appl. No.: **15/362,094**

(22) Filed: **Nov. 28, 2016**

(65) **Prior Publication Data**

US 2017/0151022 A1 Jun. 1, 2017

Related U.S. Application Data

(63) Continuation of application No. 14/171,346, filed on Feb. 3, 2014, now Pat. No. 9,504,530, which is a (Continued)

(51) **Int. Cl.**
A61B 34/20 (2016.01)
A61B 17/17 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 34/20** (2016.02); **A61B 5/062** (2013.01); **A61B 17/1615** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC **A61B 34/20**; **A61B 2034/2051**; **A61B 2034/105**; **A61B 2034/2072**; **A61B 34/10**;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,576,781 A 3/1926 Phillips
1,735,726 A 11/1929 Bornhardt
(Continued)

FOREIGN PATENT DOCUMENTS

CA 964149 3/1975
DE 3042343 A1 6/1982
(Continued)

OTHER PUBLICATIONS

“AxiEM Electromagnetic Navigation,” tri-fold brochure, Medtronic Navigation (2005) 2 pages.

(Continued)


Primary Examiner — Baisakhi Roy

(74) *Attorney, Agent, or Firm* — Harness, Dickey & Pierce, P.L.C.

(57) **ABSTRACT**

Disclosed is a surgical navigation system for tracking an instrument relative to a patient. The system can track a portion of the patient, an instrument, and/or both relative to image data, a coordinate system, an atlas, a morphed atlas, or combinations thereof. The system can include a tracking device on the instrument to provide six degree of freedom information regarding the location of the instrument.

20 Claims, 49 Drawing Sheets

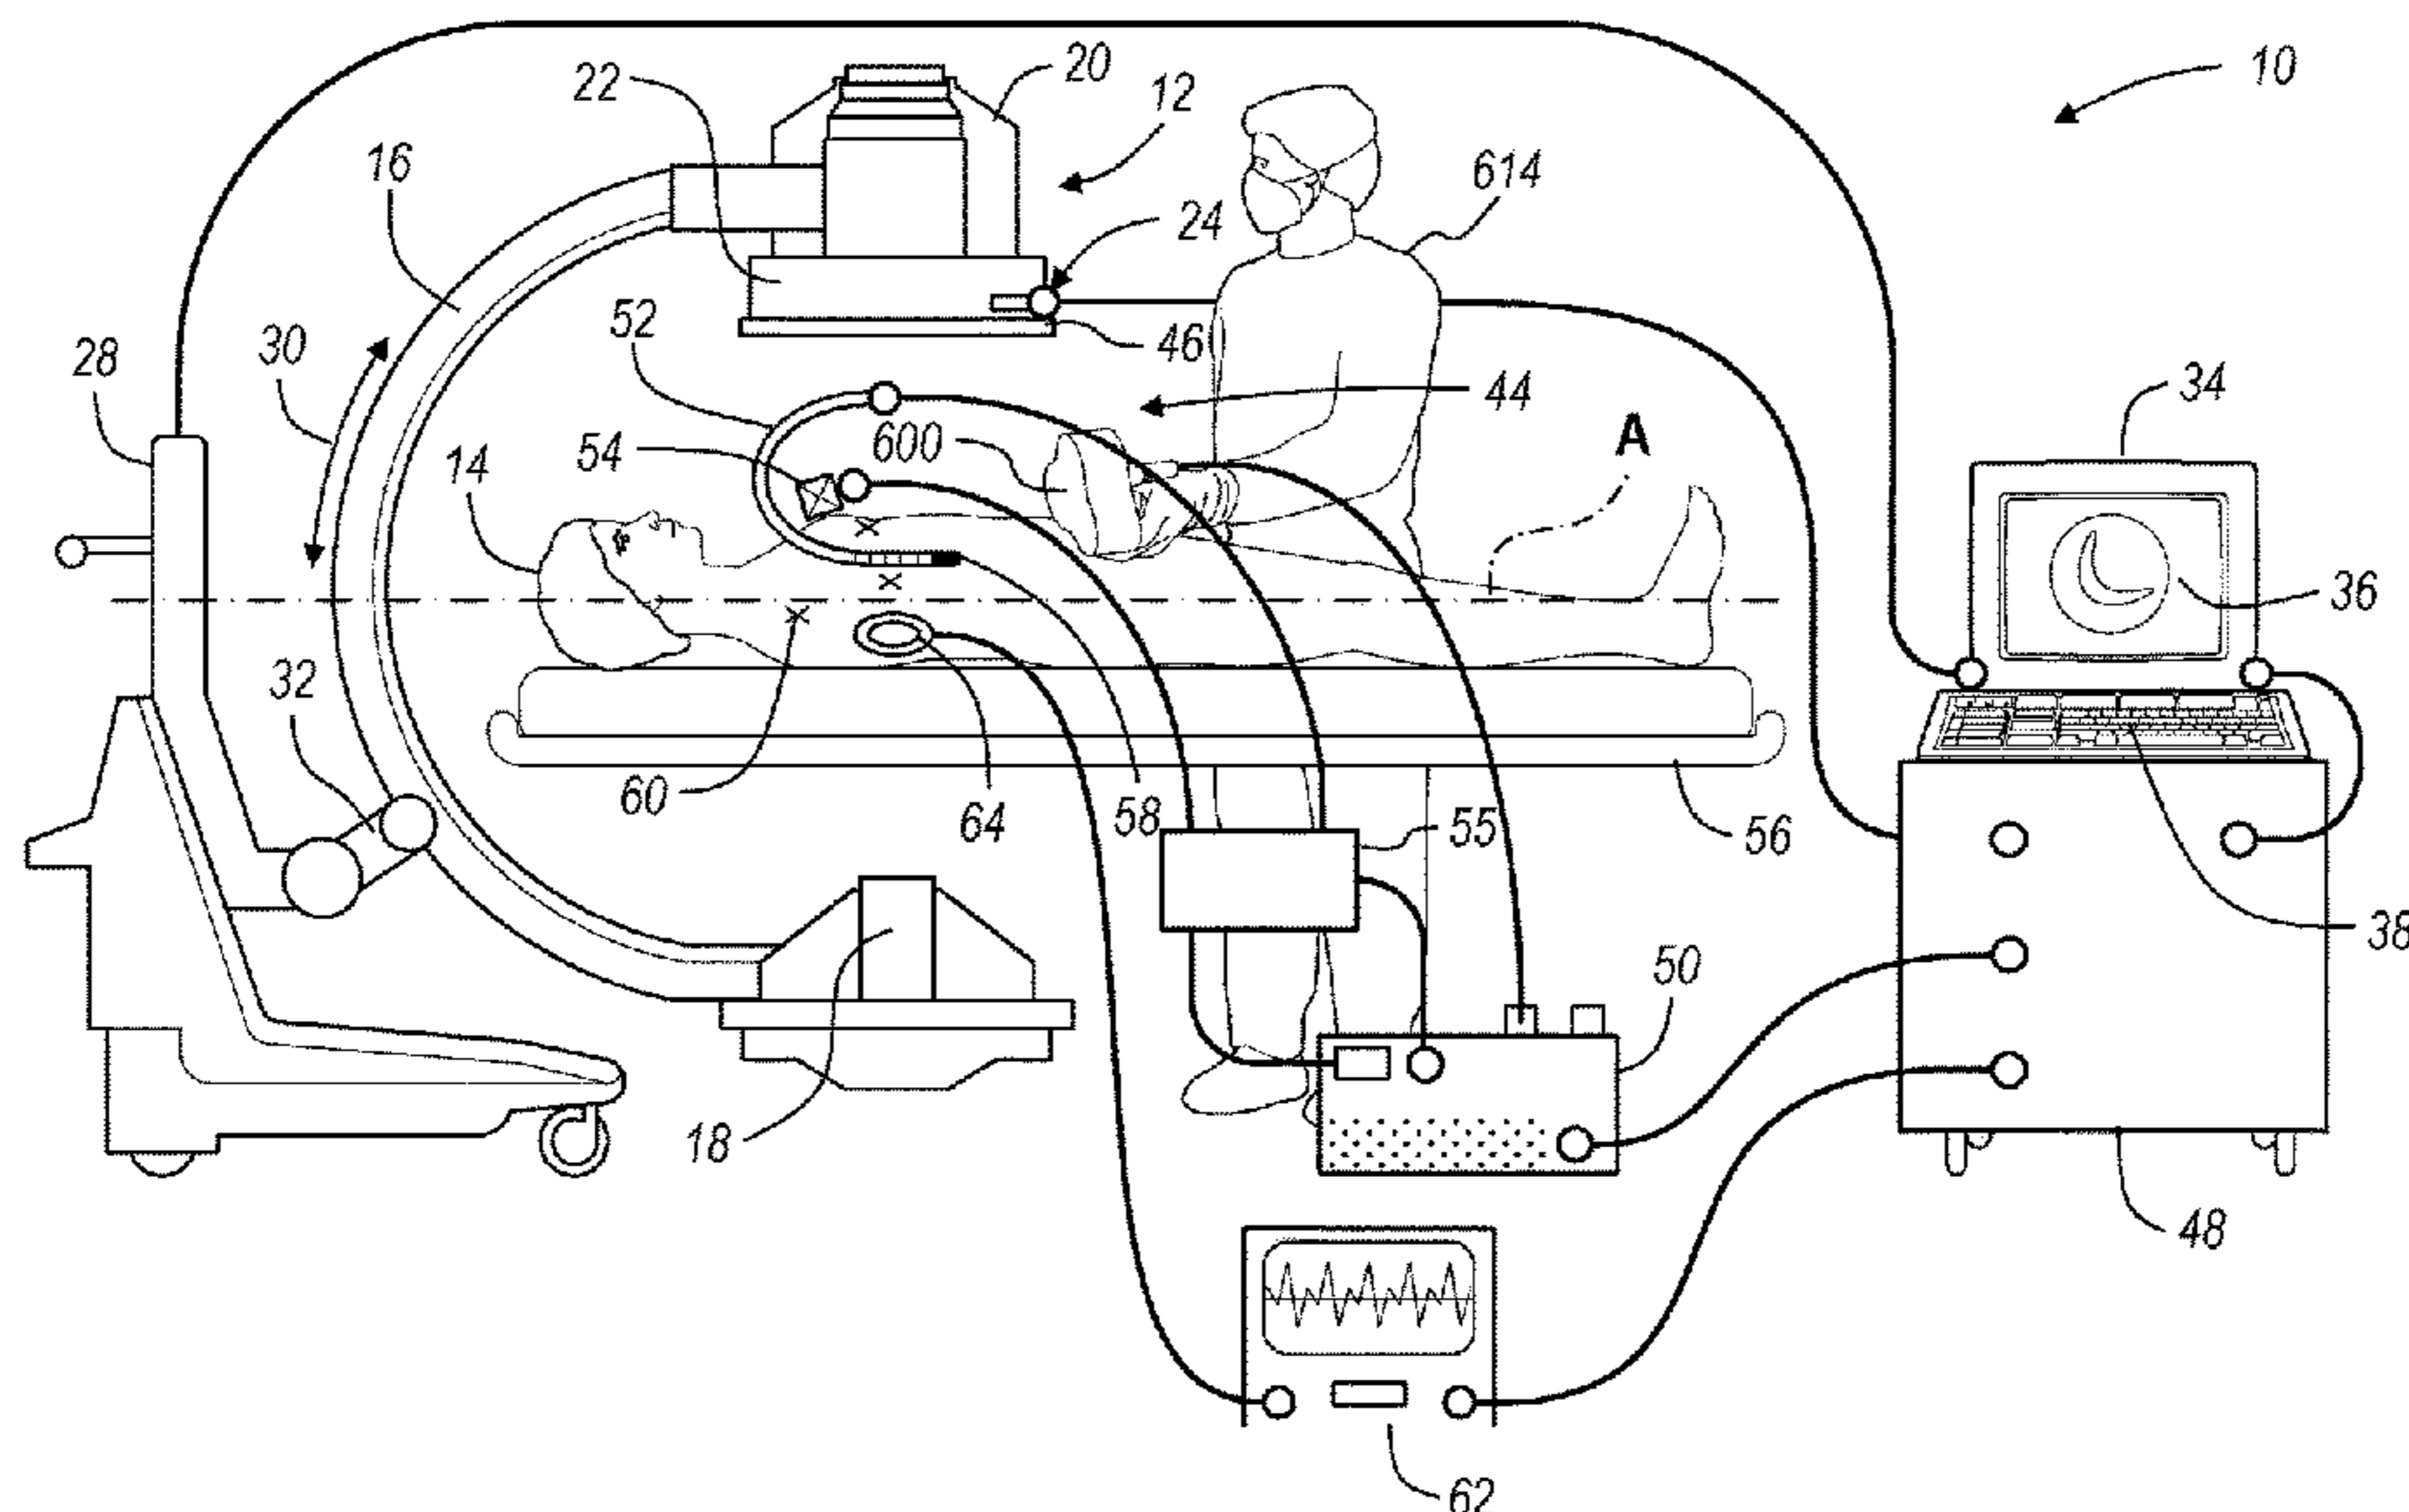

Related U.S. Application Data

continuation of application No. 12/770,181, filed on Apr. 29, 2010, now Pat. No. 8,644,907, which is a continuation-in-part of application No. 11/247,848, filed on Oct. 11, 2005, now Pat. No. 8,057,407, which is a continuation of application No. 10/289,869, filed on Nov. 7, 2002, now Pat. No. 7,007,699, which is a continuation of application No. 09/428,721, filed on Oct. 28, 1999, now Pat. No. 6,499,488, said application No. 12/770,181 is a continuation-in-part of application No. 11/179,044, filed on Jul. 11, 2005, now Pat. No. 8,239,001, which is a continuation-in-part of application No. 10/941,782, filed on Sep. 15, 2004, now Pat. No. 7,751,865, which is a continuation-in-part of application No. 10/688,068, filed on Oct. 17, 2003, now Pat. No. 7,366,562.

(51) **Int. Cl.**

A61B 17/16 (2006.01)
A61B 5/06 (2006.01)
A61B 90/00 (2016.01)
A61B 17/00 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 17/1703* (2013.01); *A61B 90/39* (2016.02); *A61B 2017/0046* (2013.01); *A61B 2017/00221* (2013.01); *A61B 2017/00477* (2013.01); *A61B 2034/2051* (2016.02); *A61B 2034/2068* (2016.02); *A61B 2034/2072* (2016.02); *A61B 2090/3983* (2016.02); *A61B 2090/3987* (2016.02)

(58) **Field of Classification Search**

CPC *A61B 17/1615*; *A61B 17/1703*; *A61B 2017/00477*

See application file for complete search history.

(56)

References Cited

U.S. PATENT DOCUMENTS

2,407,845 A 9/1946 Nemeyer
 2,650,588 A 9/1953 Drew
 2,697,433 A 12/1954 Sehnder
 3,016,899 A 1/1962 Stenvall
 3,017,887 A 1/1962 Heyer
 3,061,936 A 11/1962 Dobbeleer
 3,073,310 A 1/1963 Mocarski
 3,109,588 A 11/1963 Polhemus et al.
 3,294,083 A 12/1966 Alderson
 3,367,326 A 2/1968 Frazier
 3,439,256 A 4/1969 Kahne
 3,577,150 A 5/1971 Alden
 3,577,160 A 5/1971 White
 3,614,950 A 10/1971 Rabey
 3,644,825 A 2/1972 Davis, Jr. et al.
 3,674,014 A 7/1972 Tillander
 3,702,935 A 11/1972 Carey et al.
 3,704,707 A 12/1972 Halloran
 3,821,469 A 6/1974 Whetstone et al.
 3,868,565 A 2/1975 Kuipers
 3,941,127 A 3/1976 Froning
 3,983,474 A 9/1976 Kuipers
 4,017,858 A 4/1977 Kuipers
 4,037,592 A 7/1977 Kronner
 4,052,620 A 10/1977 Brunnett
 4,054,881 A 10/1977 Raab
 4,117,337 A 9/1978 Staats
 4,173,228 A 11/1979 Van Steenwyk et al.
 4,182,312 A 1/1980 Mushabac
 4,202,349 A 5/1980 Jones
 4,228,799 A 10/1980 Anichkov et al.
 4,256,112 A 3/1981 Kopf et al.

4,262,306 A 4/1981 Renner
 4,287,809 A 9/1981 Egli et al.
 4,298,874 A 11/1981 Kuipers
 4,314,251 A 2/1982 Raab
 4,317,078 A 2/1982 Weed et al.
 4,319,136 A 3/1982 Jinkins
 4,328,548 A 5/1982 Crow et al.
 4,328,813 A 5/1982 Ray
 4,339,953 A 7/1982 Iwasaki
 4,341,220 A 7/1982 Perry
 4,346,384 A 8/1982 Raab
 4,358,856 A 11/1982 Stivender et al.
 4,368,536 A 1/1983 Pfeiler
 4,396,885 A 8/1983 Constant
 4,396,945 A 8/1983 DiMatteo et al.
 4,403,321 A 9/1983 Kruger
 4,418,422 A 11/1983 Richter et al.
 4,419,012 A 12/1983 Stephenson et al.
 4,422,041 A 12/1983 Lienau
 4,431,005 A 2/1984 McCormick
 4,445,106 A 4/1984 Shah
 4,485,815 A 12/1984 Amplatz et al.
 4,506,676 A 3/1985 Duska
 4,543,959 A 10/1985 Sepponen
 4,548,208 A 10/1985 Niemi
 4,571,834 A 2/1986 Fraser et al.
 4,572,198 A 2/1986 Codrington
 4,583,538 A 4/1986 Onik et al.
 4,584,577 A 4/1986 Temple
 4,608,977 A 9/1986 Brown
 4,613,866 A 9/1986 Blood
 4,617,925 A 10/1986 Laitinen
 4,618,978 A 10/1986 Cosman
 4,621,628 A 11/1986 Bruderemann
 4,625,718 A 12/1986 Olerud et al.
 4,638,798 A 1/1987 Shelden et al.
 4,642,786 A 2/1987 Hansen
 4,645,343 A 2/1987 Stockdale et al.
 4,649,504 A 3/1987 Krouglicof et al.
 4,651,732 A 3/1987 Frederick
 4,653,509 A 3/1987 Oloff et al.
 4,659,971 A 4/1987 Suzuki et al.
 4,660,970 A 4/1987 Ferrano
 4,671,287 A 6/1987 Fiddian-Green
 4,673,352 A 6/1987 Hansen
 4,688,037 A 8/1987 Krieg
 4,701,049 A 10/1987 Beckman et al.
 4,705,395 A 11/1987 Hageniers
 4,705,401 A 11/1987 Addleman et al.
 4,706,665 A 11/1987 Gouda
 4,709,156 A 11/1987 Murphy et al.
 4,710,708 A 12/1987 Rorden et al.
 4,719,419 A 1/1988 Dawley
 4,722,056 A 1/1988 Roberts et al.
 4,722,336 A 2/1988 Kim et al.
 4,723,544 A 2/1988 Moore et al.
 4,727,565 A 2/1988 Ericson
 RE32,619 E 3/1988 Damadian
 4,733,969 A 3/1988 Case et al.
 4,737,032 A 4/1988 Addleman et al.
 4,737,794 A 4/1988 Jones
 4,737,921 A 4/1988 Goldwasser et al.
 4,742,356 A 5/1988 Kuipers
 4,742,815 A 5/1988 Ninan et al.
 4,743,770 A 5/1988 Lee
 4,743,771 A 5/1988 Sacks et al.
 4,745,290 A 5/1988 Frankel et al.
 4,750,487 A 6/1988 Zanetti
 4,753,528 A 6/1988 Hines et al.
 4,761,072 A 8/1988 Pryor
 4,764,016 A 8/1988 Johansson
 4,771,787 A 9/1988 Wurster et al.
 4,779,212 A 10/1988 Levy
 4,782,239 A 11/1988 Hirose et al.
 4,788,481 A 11/1988 Niwa
 4,791,934 A 12/1988 Brunnett
 4,793,355 A 12/1988 Crum et al.
 4,794,262 A 12/1988 Sato et al.
 4,797,907 A 1/1989 Anderton

(56)

References Cited

U.S. PATENT DOCUMENTS

4,803,976 A	2/1989	Frigg et al.	5,197,476 A	3/1993	Nowacki et al.
4,804,261 A	2/1989	Kirschen	5,197,965 A	3/1993	Cherry et al.
4,805,615 A	2/1989	Carol	5,198,768 A	3/1993	Keren
4,809,694 A	3/1989	Ferrara	5,198,877 A	3/1993	Schulz
4,821,200 A	4/1989	Oberg	5,207,688 A	5/1993	Carol
4,821,206 A	4/1989	Arora	5,211,164 A	5/1993	Allen
4,821,731 A	4/1989	Martinelli et al.	5,211,165 A	5/1993	Dumoulin et al.
4,822,163 A	4/1989	Schmidt	5,211,176 A	5/1993	Ishiguro et al.
4,825,091 A	4/1989	Breyer et al.	5,212,720 A	5/1993	Landi et al.
4,829,373 A	5/1989	Leberl et al.	5,214,615 A	5/1993	Bauer
4,836,778 A	6/1989	Baumrind et al.	5,219,351 A	6/1993	Teubner et al.
4,838,265 A	6/1989	Cosman et al.	5,222,499 A	6/1993	Allen et al.
4,841,967 A	6/1989	Chang et al.	5,224,049 A	6/1993	Mushabac
4,845,771 A	7/1989	Wislocki et al.	5,226,423 A	7/1993	Tenerz et al.
4,849,692 A	7/1989	Blood	5,228,442 A	7/1993	Imran
4,860,331 A	8/1989	Williams et al.	5,230,338 A	7/1993	Allen et al.
4,862,893 A	9/1989	Martinelli	5,230,623 A	7/1993	Guthrie et al.
4,869,247 A	9/1989	Howard, III et al.	5,233,990 A	8/1993	Barnea
4,875,165 A	10/1989	Fencil et al.	5,237,996 A	8/1993	Waldman et al.
4,875,478 A	10/1989	Chen	5,249,581 A	10/1993	Horbal et al.
4,884,566 A	12/1989	Mountz et al.	5,251,127 A	10/1993	Raab
4,889,526 A	12/1989	Rauscher et al.	5,251,635 A	10/1993	Dumoulin et al.
4,896,673 A	1/1990	Rose et al.	5,253,647 A	10/1993	Takahashi et al.
4,905,698 A	3/1990	Strohl, Jr. et al.	5,255,680 A	10/1993	Darrow et al.
4,923,459 A	5/1990	Nambu	5,257,636 A	11/1993	White
4,931,056 A	6/1990	Ghajar et al.	5,257,998 A	11/1993	Ota et al.
4,945,305 A	7/1990	Blood	5,261,404 A	11/1993	Mick et al.
4,945,914 A	8/1990	Allen	5,265,610 A	11/1993	Darrow et al.
4,951,653 A	8/1990	Fry et al.	5,265,611 A	11/1993	Hoening et al.
4,955,891 A	9/1990	Carol	5,269,759 A	12/1993	Hernandez et al.
4,961,422 A	10/1990	Marchosky et al.	5,271,400 A	12/1993	Dumoulin et al.
4,977,655 A	12/1990	Martinelli	5,273,025 A	12/1993	Sakiyama et al.
4,989,608 A	2/1991	Ratner	5,274,551 A	12/1993	Corby, Jr.
4,991,579 A	2/1991	Allen	5,279,309 A	1/1994	Taylor et al.
5,002,058 A	3/1991	Martinelli	5,285,787 A	2/1994	Machida
5,005,592 A	4/1991	Cartmell	5,291,199 A	3/1994	Overman et al.
5,013,317 A	5/1991	Cole et al.	5,291,889 A	3/1994	Kenet et al.
5,016,639 A	5/1991	Allen	5,295,483 A	3/1994	Nowacki et al.
5,017,139 A	5/1991	Mushabac	5,297,549 A	3/1994	Beatty et al.
5,027,818 A	7/1991	Bova et al.	5,299,253 A	3/1994	Wessels
5,030,196 A	7/1991	Inoue	5,299,254 A	3/1994	Dancer et al.
5,030,222 A	7/1991	Calandruccio et al.	5,299,288 A	3/1994	Glassman et al.
5,031,203 A	7/1991	Trecha	5,300,080 A	4/1994	Clayman et al.
5,042,486 A	8/1991	Pfeiler et al.	5,305,091 A	4/1994	Gelbart et al.
5,047,036 A	9/1991	Koutrouvelis	5,305,203 A	4/1994	Raab
5,050,608 A	9/1991	Watanabe et al.	5,306,271 A	4/1994	Zinreich et al.
5,054,492 A	10/1991	Scribner et al.	5,307,072 A	4/1994	Jones, Jr.
5,057,095 A	10/1991	Fabian	5,309,913 A	5/1994	Kormos et al.
5,059,789 A	10/1991	Salcudean	5,315,630 A	5/1994	Sturm et al.
5,078,140 A	1/1992	Kwoh	5,316,024 A	5/1994	Hirschi et al.
5,079,699 A	1/1992	Tuy et al.	5,318,025 A	6/1994	Dumoulin et al.
5,086,401 A	2/1992	Glassman et al.	5,320,111 A	6/1994	Livingston
5,094,241 A	3/1992	Allen	5,325,728 A	7/1994	Zimmerman et al.
5,097,839 A	3/1992	Allen	5,325,873 A	7/1994	Hirschi et al.
5,098,426 A	3/1992	Sklar et al.	5,329,944 A	7/1994	Fabian et al.
5,099,845 A	3/1992	Besz et al.	5,330,485 A	7/1994	Clayman et al.
5,099,846 A	3/1992	Hardy	5,333,168 A	7/1994	Fernandes et al.
5,105,829 A	4/1992	Fabian et al.	5,353,795 A	10/1994	Souza et al.
5,107,839 A	4/1992	Houdek et al.	5,353,800 A	10/1994	Pohndorf et al.
5,107,843 A	4/1992	Aarnio et al.	5,353,807 A	10/1994	DeMarco
5,107,862 A	4/1992	Fabian et al.	5,359,417 A	10/1994	Muller et al.
5,109,194 A	4/1992	Cantaloube	5,368,030 A	11/1994	Zinreich et al.
5,119,817 A	6/1992	Allen	5,371,778 A	12/1994	Yanof et al.
5,142,930 A	9/1992	Allen et al.	5,375,596 A	12/1994	Twiss et al.
5,143,076 A	9/1992	Hardy et al.	5,377,678 A	1/1995	Dumoulin et al.
5,152,288 A	10/1992	Hoening et al.	5,383,454 A	1/1995	Bucholz
5,160,337 A	11/1992	Cosman	5,385,146 A	1/1995	Goldreyer
5,161,536 A	11/1992	Vilkomerson et al.	5,385,148 A	1/1995	Lesh et al.
5,178,164 A	1/1993	Allen	5,386,828 A	2/1995	Owens et al.
5,178,621 A	1/1993	Cook et al.	5,389,101 A	2/1995	Heilbrun et al.
5,186,174 A	2/1993	Schlondorff et al.	5,391,199 A	2/1995	Ben-Haim
5,187,475 A	2/1993	Wagener et al.	5,394,457 A	2/1995	Leibinger et al.
5,188,126 A	2/1993	Fabian et al.	5,394,875 A	3/1995	Lewis et al.
5,190,059 A	3/1993	Fabian et al.	5,397,329 A	3/1995	Allen
5,193,106 A	3/1993	DeSena	5,398,684 A	3/1995	Hardy
			5,399,146 A	3/1995	Nowacki et al.
			5,400,384 A	3/1995	Fernandes et al.
			5,402,801 A	4/1995	Taylor
			5,403,321 A	4/1995	DiMarco

(56)

References Cited

U.S. PATENT DOCUMENTS

5,408,409 A	4/1995	Glassman et al.	5,617,462 A	4/1997	Spratt
5,413,573 A	5/1995	Koivukangas	5,617,857 A	4/1997	Chader et al.
5,417,210 A	5/1995	Funda et al.	5,619,261 A	4/1997	Anderton
5,419,325 A	5/1995	Dumoulin et al.	5,622,169 A	4/1997	Golden et al.
5,423,334 A	6/1995	Jordan	5,622,170 A	4/1997	Schulz
5,425,367 A	6/1995	Shapiro et al.	5,627,873 A	5/1997	Hanover et al.
5,425,382 A	6/1995	Golden et al.	5,628,315 A	5/1997	Vilsmeier et al.
5,426,683 A	6/1995	O'Farrell, Jr. et al.	5,630,431 A	5/1997	Taylor
5,426,687 A	6/1995	Goodall et al.	5,632,432 A	5/1997	Schulze et al.
5,427,097 A	6/1995	Depp	5,636,644 A	6/1997	Hart et al.
5,429,132 A	7/1995	Guy et al.	5,638,819 A	6/1997	Manwaring et al.
5,433,198 A	7/1995	Desai	5,640,170 A	6/1997	Anderson
RE35,025 E	8/1995	Anderton	5,642,395 A	6/1997	Anderton et al.
5,437,277 A	8/1995	Dumoulin et al.	5,643,268 A	7/1997	Vilsmeier et al.
5,443,066 A	8/1995	Dumoulin et al.	5,645,065 A	7/1997	Shapiro et al.
5,443,489 A	8/1995	Ben-Haim	5,646,524 A	7/1997	Gilboa
5,444,756 A	8/1995	Pai et al.	5,647,361 A	7/1997	Damadian
5,445,144 A	8/1995	Wodicka et al.	5,662,111 A	9/1997	Cosman
5,445,150 A	8/1995	Dumoulin et al.	5,664,001 A	9/1997	Tachibana et al.
5,445,166 A	8/1995	Taylor	5,674,296 A	10/1997	Bryan et al.
5,446,548 A	8/1995	Gerig et al.	5,676,673 A	10/1997	Ferre et al.
5,447,154 A	9/1995	Cinquin et al.	5,681,260 A	10/1997	Ueda et al.
5,448,610 A	9/1995	Yamamoto et al.	5,682,886 A	11/1997	Delp et al.
5,453,686 A	9/1995	Anderson	5,682,890 A	11/1997	Kormos et al.
5,456,718 A	10/1995	Szymaitis	5,690,108 A	11/1997	Chakeres
5,457,641 A	10/1995	Zimmer et al.	5,694,945 A	12/1997	Ben-Haim
5,458,718 A	10/1995	Venkitachalam	5,695,500 A	12/1997	Taylor et al.
5,464,446 A	11/1995	Dreessen et al.	5,695,501 A	12/1997	Carol et al.
5,469,847 A	11/1995	Zinreich et al.	5,696,500 A	12/1997	Diem
5,478,341 A	12/1995	Cook et al.	5,697,377 A	12/1997	Wittkamp
5,478,343 A	12/1995	Ritter	5,702,406 A	12/1997	Vilsmeier et al.
5,480,422 A	1/1996	Ben-Haim	5,711,299 A	1/1998	Manwaring et al.
5,480,439 A	1/1996	Bisek et al.	5,713,946 A	2/1998	Ben-Haim
5,483,961 A	1/1996	Kelly et al.	5,715,822 A	2/1998	Watkins et al.
5,484,437 A	1/1996	Michelson	5,715,836 A	2/1998	Kliegis et al.
5,485,849 A	1/1996	Panescu et al.	5,718,241 A	2/1998	Ben-Haim et al.
5,487,391 A	1/1996	Panescu	5,727,552 A	3/1998	Ryan
5,487,729 A	1/1996	Avellanet et al.	5,727,553 A	3/1998	Saad
5,487,757 A	1/1996	Truckai et al.	5,729,129 A	3/1998	Acker
5,490,196 A	2/1996	Rudich et al.	5,730,129 A	3/1998	Darrow et al.
5,494,034 A	2/1996	Schlondorff et al.	5,730,130 A	3/1998	Fitzpatrick et al.
5,503,416 A	4/1996	Aoki et al.	5,732,703 A	3/1998	Kalfas et al.
5,513,637 A	5/1996	Twiss et al.	5,735,278 A	4/1998	Hoult et al.
5,514,146 A	5/1996	Lam et al.	5,738,096 A	4/1998	Ben-Haim
5,515,160 A	5/1996	Schulz et al.	5,740,802 A	4/1998	Nafis et al.
5,517,990 A	5/1996	Kalfas et al.	5,740,808 A	4/1998	Panescu et al.
5,531,227 A	7/1996	Schneider	5,741,214 A	4/1998	Ouchi et al.
5,531,520 A	7/1996	Grimson et al.	5,742,394 A	4/1998	Hansen
5,542,938 A	8/1996	Avellanet et al.	5,744,953 A	4/1998	Hansen
5,543,951 A	8/1996	Moehrmann	5,748,767 A	5/1998	Raab
5,546,940 A	8/1996	Panescu et al.	5,749,362 A	5/1998	Funda et al.
5,546,949 A	8/1996	Frazin et al.	5,749,835 A	5/1998	Glantz
5,546,951 A	8/1996	Ben-Haim	5,752,513 A	5/1998	Acker et al.
5,551,429 A	9/1996	Fitzpatrick et al.	5,755,725 A	5/1998	Druais
5,558,091 A	9/1996	Acker et al.	RE35,816 E	6/1998	Schulz
5,566,581 A	10/1996	Smale et al.	5,758,667 A	6/1998	Slettenmark
5,566,681 A	10/1996	Manwaring et al.	5,762,064 A	6/1998	Polvani
5,568,384 A	10/1996	Robb et al.	5,767,669 A	6/1998	Hansen et al.
5,568,809 A	10/1996	Ben-haim	5,767,699 A	6/1998	Bosnyak et al.
5,571,109 A	11/1996	Bertagnoli	5,767,960 A	6/1998	Orman
5,572,999 A	11/1996	Funda et al.	5,769,789 A	6/1998	Wang et al.
5,573,533 A	11/1996	Strul	5,769,843 A	6/1998	Abela et al.
5,575,794 A	11/1996	Walus et al.	5,769,861 A	6/1998	Vilsmeier
5,575,798 A	11/1996	Koutrouvelis	5,772,594 A	6/1998	Barrick
5,583,909 A	12/1996	Hanover	5,772,661 A	6/1998	Michelson
5,588,430 A	12/1996	Bova et al.	5,775,322 A	7/1998	Silverstein et al.
5,590,215 A	12/1996	Allen	5,776,064 A	7/1998	Kalfas et al.
5,592,401 A *	1/1997	Kramer A63B 69/3608 340/524	5,782,765 A	7/1998	Jonkman
5,592,939 A	1/1997	Martinelli	5,787,886 A	8/1998	Kelly et al.
5,595,193 A	1/1997	Walus et al.	5,792,055 A	8/1998	McKinnon
5,596,228 A	1/1997	Anderton et al.	5,795,294 A	8/1998	Luber et al.
5,600,330 A	2/1997	Blood	5,797,849 A	8/1998	Vesely et al.
5,603,318 A	2/1997	Heilbrun et al.	5,799,055 A	8/1998	Peshkin et al.
5,611,025 A	3/1997	Lorensen et al.	5,799,099 A	8/1998	Wang et al.
			5,800,352 A	9/1998	Ferre et al.
			5,800,535 A	9/1998	Howard, III
			5,802,719 A	9/1998	O'Farrell, Jr. et al.
			5,803,089 A	9/1998	Ferre et al.
			5,807,252 A	9/1998	Hassfeld et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

			6,059,718 A	5/2000	Taniguchi et al.	
			6,063,022 A	5/2000	Ben-Haim	
			6,063,031 A *	5/2000	Cundari	A61B 5/0053 600/439
5,810,008 A	9/1998	Dekel et al.	6,071,288 A	6/2000	Carol et al.	
5,810,728 A	9/1998	Kuhn	6,073,043 A	6/2000	Schneider	
5,810,735 A	9/1998	Halperin et al.	6,076,008 A	6/2000	Bucholz	
5,820,553 A	10/1998	Hughes	6,091,981 A *	7/2000	Cundari	A61B 5/0053 600/407
5,823,192 A	10/1998	Kalend et al.				
5,823,958 A	10/1998	Truppe	6,096,050 A	8/2000	Audette	
5,828,725 A	10/1998	Levinson	6,104,944 A	8/2000	Martinelli	
5,828,770 A	10/1998	Leis et al.	6,106,464 A	8/2000	Bass et al.	
5,829,444 A	11/1998	Ferre et al.	6,106,486 A	8/2000	Tenerz et al.	
5,831,260 A	11/1998	Hansen	6,117,143 A *	9/2000	Hynes	A61B 90/11 600/429
5,833,608 A	11/1998	Acker				
5,834,759 A	11/1998	Glossop	6,118,845 A	9/2000	Simon et al.	
5,836,954 A	11/1998	Heilbrun et al.	6,122,538 A	9/2000	Sliwa, Jr. et al.	
5,840,024 A	11/1998	Taniguchi et al.	6,122,541 A	9/2000	Cosman et al.	
5,840,025 A	11/1998	Ben-Haim	6,131,396 A	10/2000	Duerr et al.	
5,843,076 A	12/1998	Webster, Jr. et al.	6,139,183 A	10/2000	Graumann	
5,848,967 A	12/1998	Cosman	6,147,480 A	11/2000	Osadchy et al.	
5,851,183 A	12/1998	Bucholz	6,149,592 A	11/2000	Yanof et al.	
5,865,846 A	2/1999	Bryan et al.	6,156,067 A	12/2000	Bryan et al.	
5,868,674 A	2/1999	Glowinski et al.	6,161,032 A	12/2000	Acker	
5,868,675 A	2/1999	Henrion et al.	6,165,181 A	12/2000	Heilbrun et al.	
5,868,789 A	2/1999	Huebner	6,167,296 A	12/2000	Shahidi	
5,871,445 A	2/1999	Bucholz	6,172,499 B1	1/2001	Ashe	
5,871,455 A	2/1999	Ueno	6,173,199 B1	1/2001	Gabriel	
5,871,487 A	2/1999	Warner et al.	6,175,756 B1	1/2001	Ferre et al.	
5,873,822 A	2/1999	Ferre et al.	6,178,345 B1	1/2001	Vilsmeier et al.	
5,882,304 A	3/1999	Ehnholm et al.	6,190,330 B1	2/2001	Harhen	
5,884,410 A	3/1999	Prinz	6,194,639 B1	2/2001	Botella et al.	
5,889,834 A	3/1999	Vilsmeier et al.	6,201,387 B1	3/2001	Govari	
5,891,034 A	4/1999	Bucholz	6,203,497 B1	3/2001	Dekel et al.	
5,891,157 A	4/1999	Day et al.	6,211,666 B1	4/2001	Acker	
5,904,691 A	5/1999	Barnett et al.	6,223,067 B1	4/2001	Vilsmeier et al.	
5,907,395 A	5/1999	Schulz et al.	6,226,548 B1	5/2001	Foley et al.	
5,913,820 A	6/1999	Bladen et al.	6,233,476 B1	5/2001	Strommer et al.	
5,920,395 A	7/1999	Schulz	6,236,875 B1	5/2001	Bucholz et al.	
5,921,992 A	7/1999	Costales et al.	6,246,231 B1	6/2001	Ashe	
5,923,727 A	7/1999	Navab	6,253,770 B1	7/2001	Acker et al.	
5,928,248 A	7/1999	Acker	6,259,942 B1	7/2001	Westermann et al.	
5,930,741 A *	7/1999	Kramer	6,273,896 B1	8/2001	Franck et al.	
			6,285,902 B1	9/2001	Kienzle, III et al.	
5,938,603 A	8/1999	Ponzi	6,298,262 B1	10/2001	Franck et al.	
5,938,694 A	8/1999	Jaraczewski et al.	6,304,769 B1	10/2001	Arenson et al.	
5,947,980 A	9/1999	Jensen et al.	6,314,310 B1	11/2001	Ben-Haim et al.	
5,947,981 A	9/1999	Cosman	6,332,089 B1	12/2001	Acker et al.	
5,950,629 A	9/1999	Taylor et al.	6,336,906 B1	1/2002	Hammarstrom et al.	
5,951,475 A	9/1999	Gueziec et al.	6,341,231 B1	1/2002	Ferre et al.	
5,951,571 A	9/1999	Audette	6,347,240 B1	2/2002	Foley et al.	
5,954,647 A	9/1999	Bova et al.	6,348,058 B1	2/2002	Melkent et al.	
5,954,796 A	9/1999	McCarty et al.	6,351,659 B1	2/2002	Vilsmeier	
5,957,844 A	9/1999	Dekel et al.	6,370,411 B1	4/2002	Osadchy et al.	
5,964,796 A	10/1999	Imran	6,381,485 B1	4/2002	Hunter et al.	
5,967,980 A	10/1999	Ferre et al.	6,424,856 B1	7/2002	Vilsmeier et al.	
5,967,982 A	10/1999	Barnett	6,427,079 B1	7/2002	Schneider et al.	
5,968,047 A	10/1999	Reed	6,427,314 B1	8/2002	Acker	
5,971,997 A	10/1999	Guthrie et al.	6,428,547 B1	8/2002	Vilsmeier et al.	
5,976,156 A	11/1999	Taylor et al.	6,432,041 B1	8/2002	Taniguchi et al.	
5,980,535 A	11/1999	Barnett et al.	6,434,415 B1	8/2002	Foley et al.	
5,983,126 A	11/1999	Wittkamp	6,437,567 B1	8/2002	Schenck et al.	
5,987,349 A	11/1999	Schulz	6,445,943 B1	9/2002	Ferre et al.	
5,987,960 A	11/1999	Messner et al.	6,447,448 B1	9/2002	Ishikawa et al.	
5,999,837 A	12/1999	Messner et al.	6,447,488 B2	9/2002	Estabrook et al.	
5,999,840 A	12/1999	Grimson et al.	6,468,265 B1 *	10/2002	Evans	A61B 34/32 600/103
6,001,130 A	12/1999	Bryan et al.				
6,002,378 A	12/1999	Harada et al.	6,470,207 B1	10/2002	Simon et al.	
6,006,126 A	12/1999	Cosman	6,474,341 B1	11/2002	Hunter et al.	
6,006,127 A	12/1999	Van Der Brug et al.	6,478,802 B2	11/2002	Kienzle, III et al.	
6,011,987 A	1/2000	Barnett	6,484,049 B1	11/2002	Seeley et al.	
6,013,087 A	1/2000	Adams et al.	6,490,475 B1	12/2002	Seeley et al.	
6,014,580 A	1/2000	Blume et al.	6,491,699 B1	12/2002	Henderson et al.	
6,016,439 A	1/2000	Acker	6,493,573 B1	12/2002	Martinelli et al.	
6,019,725 A	2/2000	Vesely et al.	6,498,944 B1 *	12/2002	Ben-Haim	A61B 5/0215 600/407
6,021,343 A	2/2000	Foley et al.				
6,024,408 A	2/2000	Bello et al.	6,499,488 B1 *	12/2002	Hunter	A61B 90/39 128/899
6,024,695 A	2/2000	Taylor et al.				
6,050,724 A	4/2000	Schmitz et al.	6,516,046 B1	2/2003	Frohlich et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

6,527,443 B1 3/2003 Vilsmeier et al.
 6,551,325 B2 4/2003 Neubauer et al.
 6,572,624 B2 6/2003 U et al.
 6,584,174 B2 6/2003 Schubert et al.
 6,609,022 B2 8/2003 Vilsmeier et al.
 6,611,700 B1 8/2003 Vilsmeier et al.
 6,640,128 B2 10/2003 Vilsmeier et al.
 6,694,162 B2 2/2004 Hartlep
 6,701,179 B1 3/2004 Martinelli et al.
 6,796,963 B2 9/2004 Carpenter et al.
 6,887,247 B1* 5/2005 Couture A61B 17/1703
 408/72 R
 6,926,674 B2 8/2005 Tenerz et al.
 6,951,549 B1 10/2005 Beyerlein
 6,977,575 B2 12/2005 Bernier
 7,007,699 B2 3/2006 Martinelli et al.
 7,152,608 B2 12/2006 Hunter et al.
 7,366,562 B2 4/2008 Dukesherer et al.
 7,693,757 B2* 4/2010 Zimmerman G05D 1/0246
 705/28
 7,697,972 B2 4/2010 Verard et al.
 7,751,865 B2 7/2010 Jascob et al.
 7,818,044 B2 10/2010 Dukesherer et al.
 7,840,253 B2 11/2010 Tremblay et al.
 7,966,057 B2 6/2011 Macaulay et al.
 7,971,341 B2 7/2011 Dukesherer et al.
 8,057,407 B2 11/2011 Martinelli et al.
 8,239,001 B2 8/2012 Verard et al.
 8,271,069 B2 9/2012 Jascob et al.
 8,359,730 B2 1/2013 Burg et al.
 8,549,732 B2 10/2013 Burg et al.
 8,644,907 B2 2/2014 Hartmann et al.
 2001/0007918 A1 7/2001 Vilsmeier et al.
 2001/0044578 A1 11/2001 Ben-Haim et al.
 2002/0087101 A1 7/2002 Barrick et al.
 2002/0095081 A1 7/2002 Vilsmeier
 2002/0147497 A1 10/2002 Belef et al.
 2003/0009169 A1 1/2003 Young et al.
 2003/0066538 A1 4/2003 Martinelli et al.
 2003/0069588 A1 4/2003 Vilsmeier et al.
 2003/0078003 A1 4/2003 Hunter et al.
 2003/0097061 A1 5/2003 Ferre et al.
 2003/0114778 A1 6/2003 Vilsmeier et al.
 2003/0184285 A1 10/2003 Anderson et al.
 2003/0187347 A1 10/2003 Nevo et al.
 2004/0024309 A1 2/2004 Ferre et al.
 2004/0097805 A1 5/2004 Verard et al.
 2004/0199071 A1 10/2004 Lardo et al.
 2004/0215071 A1 10/2004 Frank et al.
 2005/0075632 A1 4/2005 Russell et al.
 2005/0085715 A1 4/2005 Dukesherer et al.
 2005/0085720 A1 4/2005 Jascob et al.
 2005/0104776 A1 5/2005 Anderson
 2005/0105212 A1 5/2005 Sato
 2005/0107882 A1 5/2005 Stone et al.
 2005/0215887 A1* 9/2005 Ben-Haim A61B 18/20
 600/424
 2005/0245817 A1 11/2005 Clayton et al.
 2006/0025668 A1 2/2006 Peterson et al.
 2006/0025677 A1 2/2006 Verard et al.
 2006/0036189 A1 2/2006 Martinelli et al.
 2006/0084867 A1 4/2006 Tremblay et al.
 2006/0190009 A1* 8/2006 Revie A61B 34/20
 606/129
 2007/0016006 A1 1/2007 Shachar
 2007/0052507 A1* 3/2007 Zaitso H01F 41/098
 335/216
 2007/0164900 A1* 7/2007 Schneider A61B 34/20
 342/357.75
 2007/0283773 A1* 12/2007 Baldewein A61B 90/39
 73/866.5
 2008/0033282 A1 2/2008 Bar-Tal et al.
 2008/0171937 A1 7/2008 Dukesherer et al.
 2008/0172069 A1 7/2008 Dukesherer et al.

2008/0269596 A1* 10/2008 Revie A61F 2/4603
 600/424
 2009/0115406 A1 5/2009 Anderson et al.
 2009/0264863 A1* 10/2009 Bloom A61M 25/0068
 604/524
 2009/0290771 A1 11/2009 Frank et al.
 2010/0210939 A1 8/2010 Hartmann et al.
 2010/0274124 A1 10/2010 Jascob et al.
 2010/0312096 A1* 12/2010 Guttman A61B 34/10
 600/411
 2011/0160568 A1* 6/2011 Seeley A61B 34/20
 600/424
 2011/0258842 A1 10/2011 Dukesherer et al.
 2011/0258843 A1 10/2011 Dukesherer et al.
 2014/0148692 A1 5/2014 Hartmann et al.

FOREIGN PATENT DOCUMENTS

DE 3508730 9/1986
 DE 3717871 12/1988
 DE 3831278 A1 3/1989
 DE 3838011 7/1989
 DE 4213426 A1 10/1992
 DE 4225112 C1 12/1993
 DE 4233978 C1 4/1994
 DE 19631303 2/1998
 DE 19715202 A1 10/1998
 DE 19751761 A1 10/1998
 DE 19832296 2/1999
 DE 19747427 A1 5/1999
 DE 10085137 11/2002
 DE 20311919 U1 10/2003
 DE 10335388 2/2005
 DE 102009030731 A1 12/2010
 EP 0062941 10/1982
 EP 0119660 9/1984
 EP 0155857 A2 9/1985
 EP 0319844 A1 6/1989
 EP 0326768 8/1989
 EP 0350996 A1 11/1990
 EP 0419729 A1 4/1991
 EP 0427358 5/1991
 EP 0456103 11/1991
 EP 0469966 A1 12/1992
 EP 0581704 12/1994
 EP 0651968 5/1995
 EP 0655138 5/1995
 EP 0908146 4/1999
 EP 0910278 A1 4/1999
 EP 0930046 7/1999
 EP 0894473 A2 12/1999
 EP 1523951 A2 4/2005
 EP 1552795 A1 7/2005
 EP 1658818 A1 5/2006
 EP 1806756 A2 7/2007
 EP 2123220 A1 11/2009
 FR 2417970 9/1979
 FR 2618211 B1 11/1991
 GB 2094590 9/1982
 GB 2164856 A 4/1986
 JP 6194639 A 10/1984
 JP S62-327 A 11/1987
 JP 63240851 A 10/1988
 JP 2765738 T 4/1991
 JP 3267054 11/1991
 WO WO-8809151 12/1988
 WO WO-8905123 A1 6/1989
 WO WO-9005494 A1 5/1990
 WO WO-9103982 4/1991
 WO WO-9104711 4/1991
 WO WO-9107726 A1 5/1991
 WO WO-9203090 3/1992
 WO WO-9206645 A1 4/1992
 WO WO-9404938 A1 3/1994
 WO WO-9423647 10/1994
 WO WO-9424933 11/1994
 WO WO-9507055 3/1995
 WO WO-96/05768 A 2/1996

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO-9611624	A2	4/1996
WO	WO-9632059	A1	10/1996
WO	WO-9632060	A1	10/1996
WO	WO-9729683	A1	8/1997
WO	WO-9729684	A1	8/1997
WO	WO-9729710	A1	8/1997
WO	WO-9736192	A1	10/1997
WO	WO-9749453	A1	12/1997
WO	WO-9808554		3/1998
WO	WO-9838908		9/1998
WO	WO-9915097		4/1999
WO	WO-9921498	A1	5/1999
WO	WO-9923956		5/1999
WO	WO-9926549		6/1999
WO	WO-9929253		6/1999
WO	WO-9933406		7/1999
WO	WO-9937208	A1	7/1999
WO	WO-9938449		8/1999
WO	WO-99/27839	A9	10/1999
WO	WO-9952094		10/1999
WO	WO-9960939		12/1999
WO	WO-0130257		5/2001
WO	WO-0130437		5/2001
WO	WO-03002012	A1	1/2003
WO	2006096685	A1	9/2006

OTHER PUBLICATIONS

"Prestige Cervical Disc System Surgical Technique", 12 pgs., undated.

Adams et al., "Orientation Aid for Head and Neck Surgeons," *Innov. Tech. Biol. Med.*, vol. 13, No. 4, 1992, pp. 409-424.

Adams et al., *Computer-Assisted Surgery*, IEEE Computer Graphics & Applications, pp. 43-51, (May 1990).

Barrick et al., "Prophylactic Intramedullary Fixation of the Tibia for Stress Fracture in a Professional Athlete," *Journal of Orthopaedic Trauma*, vol. 6, No. 2, pp. 241-244 (1992).

Barrick et al., "Technical Difficulties with the Brooker-Wills Nail in Acute Fractures of the Femur," *Journal of Orthopaedic Trauma*, vol. 6, No. 2, pp. 144-150 (1990).

Barrick, "Distal Locking Screw Insertion Using a Cannulated Drill Bit: Technical Note," *Journal of Orthopaedic Trauma*, vol. 7, No. 3, 1993, pp. 248-251.

Batnitzky et al., "Three-Dimensional Computer Reconstructions of Brain Lesions from Surface Contours Provided by Computed Tomography: A Prospectus," *Neurosurgery*, vol. 11, No. 1, Part 1, 1982, pp. 73-84.

Benzel et al., "Magnetic Source Imaging: a Review of the Magnes System of Biomagnetic Technologies Incorporated," *Neurosurgery*, vol. 33, No. 2 (Aug. 1993), pp. 252-259.

Bergstrom et al. *Stereotaxic Computed Tomography*, *Am. J. Roentgenol.*, vol. 127 pp. 167-170 (1976).

Bouazza-Marouf et al.; "Robotic-Assisted Internal Fixation of Femoral Fractures", *IMECHE.*, pp. 51-58 (1995).

Brack et al., "Accurate X-ray Based Navigation in Computer-Assisted Orthopedic Surgery," *CAR '98*, pp. 716-722.

Brown, R., M.D., *A Stereotactic Head Frame for Use with CT Body Scanners*, *Investigative Radiology*. Copyright. J.B. Lippincott Company, pp. 300-304 (Jul.-Aug. 1979).

Bryan, "Bryan Cervical Disc System Single Level Surgical Technique", *Spinal Dynamics*, 2002, pp. 1-33.

Bucholz et al., "Variables affecting the accuracy of stereotactic localization using computerized tomography," *Journal of Neurosurgery*, vol. 79, Nov. 1993, pp. 667-673.

Bucholz, R.D., et al. *Image-guided surgical techniques for infections and trauma of the central nervous system*, *Neurosurg. Clinics of N.A.*, vol. 7, No. 2, pp. 187-200 (1996).

Bucholz, R.D., et al., *A Comparison of Sonic Digitizers Versus Light Emitting Diode-Based Localization*, *Interactive Image-Guided Neurosurgery*, Chapter 16, pp. 179-200 (1993).

Bucholz, R.D., et al., *Intraoperative localization using a three dimensional optical digitizer*, *SPIE—The Intl. Soc. for Opt. Eng.*, vol. 1894, pp. 312-322 (Jan. 17-19, 1993).

Bucholz, R.D., et al., *The Correction of Stereotactic Inaccuracy Caused by Brain Shift Using an Intraoperative Ultrasound Device*, *First Joint Conference, Computer Vision, Virtual Reality and Robotics in Medicine and Medical Robotics and Computer-Assisted Surgery*, Grenoble, France, pp. 459-466 (Mar. 19-22, 1997).

Champleboux et al., "Accurate Calibration of Cameras and Range Imaging Sensors: the NPBS Method," *IEEE International Conference on Robotics and Automation*, Nice, France, May 1992.

Champleboux, "Utilisation de Fonctions Splines pour la Mise au Point D'un Capteur Tridimensionnel sans Contact," *Quelques Applications Medicales*, Jul. 1991.

Cinquin et al., "Computer Assisted Medical Interventions," *IEEE Engineering in Medicine and Biology*, May/Jun. 1995, pp. 254-263.

Cinquin et al., "Computer Assisted Medical Interventions," *International Advanced Robotics Programme*, Sep. 1989, pp. 63-65.

Clarysse et al., "A Computer-Assisted System for 3-D Frameless Localization in Stereotaxic MRI," *IEEE Transactions on Medical Imaging*, vol. 10, No. 4, Dec. 1991, pp. 523-529.

Communication pursuant to Article 94(3) EPC dated Oct. 6, 2016 for European Application No. 11717425.0-1659 corresponding to PCT/US2011/0133163 which claims benefit of U.S. Appl. No. 12/770,181, filed Apr. 20, 2010.

Cutting M.D. et al., *Optical Tracking of Bone Fragments During Craniofacial Surgery*, *Second Annual International Symposium on Medical Robotics and Computer Assisted Surgery*, pp. 221-225, (Nov. 1995).

European Office Action dated Nov. 24, 2010 for EP1523951 claiming benefit of U.S. Appl. No. 10/941,782, filed Sep. 15, 2004 and U.S. Appl. No. 10/941,782, filed Sep. 15, 2004.

European Search Report completed Jul. 6, 2005 for European Application No. EP 04 02 4680.

European Search Report dated Feb. 23, 2011 for EP10183063 which claims benefit of European Serial No. 040246803 filed Oct. 15, 2004; which claims benefit of U.S. Appl. No. 10/941,782, filed Sep. 15, 2004 and U.S. Appl. No. 10/688,068, filed Oct. 17, 2003.

European Search Report dated Nov. 29, 2010 for European Application No. EP10183240 claiming benefit of EPSN 04024680.3, filed Oct. 15, 2004; which claims benefit of U.S. Appl. No. 10/941,782, filed Sep. 15, 2004; which claims benefit of U.S. Appl. No. 10/688,068, filed Oct. 17, 2003.

Extended Search Report dated May 4, 2016 for European Application No. 15197256.9-1654.

Feldmar et al., "3D-2D Projective Registration of Free-Form Curves and Surfaces," *Rapport de recherche (Inria Sophia Antipolis)*, 1994, pp. 1-44.

Foley et al., "Fundamentals of Interactive Computer Graphics," *The Systems Programming Series*, Chapter 7, Jul. 1984, pp. 245-266.

Foley et al., "Image-guided Intraoperative Spinal Localization," *Intraoperative Neuroprotection*, Chapter 19, 1996, pp. 325-340.

Foley, "The StealthStation: Three-Dimensional Image-Interactive Guidance for the Spine Surgeon," *Spinal Frontiers*, Apr. 1996, pp. 7-9.

Friets, E.M., et al. *A Frameless Stereotaxic Operating Microscope for Neurosurgery*, *IEEE Trans. on Biomed. Eng.*, vol. 36, No. 6, pp. 608-617 (Jul. 1989).

Gallen, C.C., et al., *Intracranial Neurosurgery Guided by Functional Imaging*, *Surg. Neurol.*, vol. 42, pp. 523-530 (1994).

Galloway, R.L., et al., *Interactive Image-Guided Neurosurgery*, *IEEE Trans. on Biomed. Eng.*, vol. 89, No. 12, pp. 1226-1231 (1992).

Galloway, R.L., Jr. et al., *Optical localization for interactive image-guided neurosurgery*, *SPIE*, vol. 2164, pp. 137-145 (undated, the date is May 1, 1994).

German Office Action dated Jan. 5, 2009 for German Publication No. 100851371 claiming benefit of PCT/US00/29880, filed Oct. 27, 2000; which claims priority of U.S. Appl. No. 09/428,721, filed Oct. 28, 1999.

Germano, "Instrumentation, Technique and Technology", *Neurosurgery*, vol. 37, No. 2, Aug. 1995, pp. 348-350.

(56)

References Cited

OTHER PUBLICATIONS

- Gildenberg et al., "Calculation of Stereotactic Coordinates from the Computed Tomographic Scan," *Neurosurgery*, vol. 10, No. 5, May 1982, pp. 580-586.
- Gomez, C.R., et al., *Transcranial Doppler Ultrasound Following Closed Head Injury: Vasospasm or Vasoparalysis?*, *Surg. Neurol.*, vol. 35, pp. 30-35 (1991).
- Gonzalez, "Digital Image Fundamentals," *Digital Image Processing*, Second Edition, 1987, pp. 52-54.
- Gottesfeld Brown et al., "Registration of Planar Film Radiographs with Computer Tomography," *Proceedings of MMBIA*, Jun. 1996, pp. 42-51.
- Grimson, W.E.L., *An Automatic Registration Method for Frameless Stereotaxy, Image Guided Surgery, and enhanced Reality Visualization*, IEEE, pp. 430-436 (1994).
- Grimson, W.E.L., et al., *Virtual-reality technology is giving surgeons the equivalent of x-ray vision helping them to remove tumors more effectively, to minimize surgical wounds and to avoid damaging critical tissues*, *Sci. Amer.*, vol. 280, No. 6, pp. 62-69 (Jun. 1999).
- Guezic et al., "Registration of Computed Tomography Data to a Surgical Robot Using Fluoroscopy: A Feasibility Study," *Computer Science/Mathematics*, Sep. 27, 1996, 6 pages.
- Guthrie, B.L., *Graphic-Interactive Cranial Surgery: The Operating Ann System*, *Handbook of Stereotaxy Using the CRW Apparatus*, Chapter 13, pp. 193-211, undated.
- Hamadeh et al., "Kinematic Study of Lumbar Spine Using Functional Radiographies and 3D/2D Registration," *TIMC UMR 5525—IMAG*, 1997.
- Hamadeh et al., "Automated 3-Dimensional Computed Tomographic and Fluoroscopic Image Registration," *Computer Aided Surgery* (1998), 3:11-19.
- Hamadeh et al., "Towards Automatic Registration Between CT and X-ray Images: Cooperation Between 3D/2D Registration and 2D Edge Detection," *MRCAS '95*, pp. 39-46.
- Hardy, T., M.D., et al., *CASS: A Program for Computer Assisted Stereotaxic Surgery*, *The Fifth Annual Symposium on Computer Applications in Medical Care*, Proceedings, Nov. 1-4, 1981, IEEE, pp. 1116-1126, (1981).
- Hatch, "Reference-Display System for the Integration of CT Scanning and the Operating Microscope," *Thesis, Thayer School of Engineering*, Oct. 1984, pp. 1-189.
- Hatch, et al., "Reference-Display System for the Integration of CT Scanning and the Operating Microscope," *Proceedings of the Eleventh Annual Northeast Bioengineering Conference*, Mar. 14-15, 1985, pp. 252-254.
- Heilbrun et al., "Preliminary experience with Brown-Roberts-Wells (BRW) computerized tomography stereotaxic guidance system," *Journal of Neurosurgery*, vol. 59, Aug. 1983, pp. 217-222.
- Heilbrun, M.D., *Progressive Technology Applications, Neurosurgery for the Third Millennium*, Chapter 15, J. Whitaker & Sons, Ltd., Amer. Assoc. of Neurol. Surgeons, pp. 191-198 (1992).
- Heilbrun, M.P., *Computed Tomography—Guided Stereotactic Systems*, *Clinical Neurosurgery*, Chapter 31, pp. 564-581 (1983).
- Heilbrun, M.P., et al., *Stereotactic Localization and Guidance Using a Machine Vision Technique*, *Stereotact & Funct. Neurosurg.*, *Proceed. of the Mtg. of the Amer. Soc. for Sterot. and Funct. Neurosurg.* (Pittsburgh, PA) vol. 58, pp. 94-98 (1992).
- Henderson et al., "An Accurate and Ergonomic Method of Registration for Image-guided Neurosurgery," *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, Jul.-Aug. 1994, pp. 273-277.
- Hoerenz, "The Operating Microscope I. Optical Principles, Illumination Systems, and Support Systems," *Journal of Microsurgery*, vol. 1, 1980, pp. 364-369.
- Hofstetter et al., "Fluoroscopy Based Surgical Navigation—Concept and Clinical Applications," *Computer Assisted Radiology and Surgery*, 1997, pp. 956-960.
- Horner et al., "A Comparison of CT-Stereotaxic Brain Biopsy Techniques," *Investigative Radiology*, Sep.-Oct. 1984, pp. 367-373.
- Hounsfield, "Computerized transverse axial scanning (tomography): Part 1. Description of system," *British Journal of Radiology*, vol. 46, No. 552, Dec. 1973, pp. 1016-1022.
- International Search Report and Written Opinion dated Jul. 19, 2011 for PCT/US2011/033163 which claims benefit of U.S. Appl. No. 12/770,181, filed Apr. 20, 2010.
- Jacques et al., "Computerized three-dimensional stereotaxic removal of small central nervous system lesion in patients," *J. Neurosurg.*, vol. 53, Dec. 1980, pp. 816-820.
- Joskowicz et al., "Computer-Aided Image-Guided Bone Fracture Surgery: Concept and Implementation," *CAR '98*, pp. 710-715.
- Kall, B., *The Impact of Computer and Imaging Technology on Stereotactic Surgery*, *Proceedings of the Meeting of the American Society for Stereotactic and Functional Neurosurgery*, pp. 10-22 (1987).
- Kato, A., et al., *A frameless, armless navigational system for computer-assisted neurosurgery*, *J. Neurosurg.*, vol. 74, pp. 845-849 (May 1991).
- Kelly et al., "Computer-assisted stereotaxic laser resection of intra-axial brain neoplasms," *Journal of Neurosurgery*, vol. 64, Mar. 1986, pp. 427-439.
- Kelly et al., "Precision Resection of Intra-Axial CNS Lesions by CT-Based Stereotactic Craniotomy and Computer Monitored CO2 Laser," *Acta Neurochirurgica*, vol. 68, 1983, pp. 1-9.
- Kelly, P.J., *Computer-Directed Stereotactic Resection of Brain Tumors*, *Neurologica Operative Atlas*, vol. 1, No. 4, pp. 299-313 (1991).
- Kelly, P.J., et al., *Results of Computed Tomography-based Computer-assisted Stereotactic Resection of Metastatic Intracranial Tumors*, *Neurosurgery*, vol. 22, No. 1, Part 1, 1988, pp. 7-17 (Jan. 1988).
- Kelly, P.J., *Stereotactic Imaging, Surgical Planning and Computer-Assisted Resection of Intracranial Lesions: Methods and Results*, *Advances and Technical Standards in Neurosurgery*, vol. 17, pp. 78-118, (1990).
- Kim, W.S. et al., *A Helmet Mounted Display for Telerobotics*, IEEE, pp. 543-547 (1988).
- Klimek, L., et al., *Long-Term Experience with Different Types of Localization Systems in Skull-Base Surgery, Ear, Nose & Throat Surgery*, Chapter 51, pp. 635-638 (undated), 1996.
- Kosugi, Y., et al., *An Articulated Neurosurgical Navigation System Using MRI and CT Images*, *IEEE Trans. on Biomed. Eng.* vol. 35, No. 2, pp. 147-152 (Feb. 1988).
- Krybus, W., et al., *Navigation Support for Surgery by Means of Optical Position Detection*, *Computer Assisted Radiology Proceed. of the Intl. Symp. CAR '91 Computed Assisted Radiology*, pp. 362-366 (Jul. 3-6, 1991).
- Kwoh, Y.S., Ph.D., et al., *A New Computerized Tomographic-Aided Robotic Stereotaxis System*, *Robotics Age*, vol. 7, No. 6, pp. 17-22 (Jun. 1985).
- Laitinen et al., "An Adapter for Computed Tomography-Guided, Stereotaxis," *Surg. Neurol.*, 1985, pp. 559-566.
- Laitinen, "Noninvasive multipurpose stereoadapter," *Neurological Research*, Jun. 1987, pp. 137-141.
- Lavallee et al., "Matching 3-D Smooth Surfaces with their 2-D Projections using 3-D Distance Maps," *SPIE*, vol. 1570, *Geometric Methods in Computer Vision*, 1991, pp. 322-336.
- Lavallee et al., "Computer Assisted Driving of a Needle into the Brain," *Proceedings of the International Symposium CAR '89, Computer Assisted Radiology*, 1989, pp. 416-420.
- Lavallee et al., "Computer Assisted Interventionist Imaging: The Instance of Stereotactic Brain Surgery," *North-Holland MEDINFO 89, Part 1*, 1989, pp. 613-617.
- Lavallee et al., "Computer Assisted Spine Surgery: A Technique for Accurate Transpedicular Screw Fixation Using CT Data and a 3-D Optical Localizer," *TIMC, Faculte de Medecine de Grenoble* (1995).
- Lavallee et al., "Image guided operating robot: a clinical application in stereotactic neurosurgery," *Proceedings of the 1992 IEEE International Conference on Robotics and Automation*, May 1992, pp. 618-624.
- Lavallee et al., "Matching of Medical Images for Computed and Robot Assisted Surgery," *IEEE EMBS*, Orlando, 1991.

(56)

References Cited

OTHER PUBLICATIONS

- Lavallee, "A New System for Computer Assisted Neurosurgery," IEEE Engineering in Medicine & Biology Society 11th Annual International Conference, 1989, pp. 0926-0927.
- Lavallee, "VI Adaptation de la Methodologie a Quelques Applications Cliniques," Chapitre VI, pp. 133-148.
- Lavallee, S., et al., Computer Assisted Knee Anterior Cruciate Ligament Reconstruction First Clinical Tests, Proceedings of the First International Symposium on Medical Robotics and Computer Assisted Surgery, pp. 11-16 (Sep. 1994).
- Lavallee, S., et al., Computer Assisted Medical Interventions, NATO ASI Series, vol. F 60, 3d Imaging in Medic., pp. 301-312 (1990).
- Leavitt, D.D., et al., Dynamic Field Shaping to Optimize Stereotactic Radiosurgery, I.J. Rad. Onc. Biol. Phys., vol. 21, pp. 1247-1255 (1991).
- Leksell et al., "Stereotaxis and Tomography—A Technical Note," ACTA Neurochirurgica, vol. 52, 1980, pp. 1-7.
- Lemieux et al., "A Patient-to-Computed-Tomography Image Registration Method Based on Digitally Reconstructed Radiographs," Med. Phys. 21 (11), Nov. 1994, pp. 1749-1760.
- Levin et al., "The Brain: Integrated Three-dimensional Display of MR and PET Images," Radiology, vol. 172, No. 3, Sep. 1989, pp. 783-789.
- Maurer, Jr., et al., Registration of Head CT Images to Physical Space Using a Weighted Combination of Points and Surfaces, IEEE Trans. on Med. Imaging, vol. 17, No. 5, pp. 753-761 (Oct. 1998).
- Mazier et al., "Computer-Assisted Interventionist Imaging: Application to the Vertebral Column Surgery," Annual International Conference of the IEEE Engineering in Medicine and Biology Society, vol. 12, No. 1, 1990, pp. 0430-0431.
- Mazier et al., Chirurgie de la Colonne Vertebrale Assiste par Ordinateur: Application au Vissage Pediculaire, Innov. Tech. Biol. Med., vol. 11, No. 5, 1990, pp. 559-566.
- McGirr, S., M.D., et al., Stereotactic Resection of Juvenile Pilocytic Astrocytomas of the Thalamus and Basal Ganglia, Neurosurgery, vol. 20, No. 3, pp. 447-452, (1987).
- Medtronic Navigation, "StealthStation.RTM. AXIEM.TM. Electromagnetic Navigation . . .", 2005, www.stealthstation.com/physician/spine/library/axiem.sub.--ent.jsp, printed Aug. 19, 2006 (2 pages).
- Merloz, et al., "Computer Assisted Spine Surgery", Clinical Assisted Spine Surgery, No. 337, pp. 86-96, 1997.
- Ng, W.S. et al., Robotic Surgery—A First-Hand Experience in Transurethral Resection of the Prostate Surgery, IEEE Eng. in Med. and Biology, pp. 120-125 (Mar. 1993).
- Partial European Search Report completed Mar. 16, 2005 for European Application No. EP 04 02 4680.
- Partial European Search Report completed Nov. 26, 2007 for European Application No. EP 06 11 6892.
- Partial European Search Report completed Nov. 8, 2006 for European Application No. EP 06 11 6892.
- Pelizzari et al., "Accurate Three-Dimensional Registration of CT, PET, and/or MR Images of the Brain," Journal of Computer Assisted Tomography, Jan./Feb. 1989, pp. 20-26.
- Pelizzari et al., "Interactive 3D Patient-Image Registration," Information Processing in Medical Imaging, 12th International Conference, IPMI '91, Jul. 7-12, 133-141 (A.C.F. Colchester et al. eds. 1991).
- Pelizzari et al., No. 528—"Three Dimensional Correlation of PET, CT and MRI Images," The Journal of Nuclear Medicine, vol. 28, No. 4, Apr. 1987, p. 682.
- Penn, R.D., et al., Stereotactic Surgery with Image Processing of Computerized Tomographic Scans, Neurosurgery, vol. 3, No. 2, pp. 157-163 (Sep.-Oct. 1978).
- Phillips et al., "Image Guided Orthopaedic Surgery Design and Analysis," Trans Inst. MC, vol. 17, No. 5, 1995, pp. 251-264.
- Pixsys, 3-D Digitizing Accessories, by Pixsys (marketing brochure)(undated) (2 pages).
- Potamianos et al., "Intra-Operative Imaging Guidance for Keyhole Surgery Methodology and Calibration," First International Symposium on Medical Robotics and Computer Assisted Surgery, Sep. 22-24, 1994, pp. 98-104.
- Reinhardt et al., "CT-Guided 'Real Time' Stereotaxy," ACTA Neurochirurgica, 1989. (2 pages).
- Reinhardt, H., et al., A Computer-Assisted Device for Intraoperative CT-Correlated Localization of Brain Tumors, pp. 51-58 (1988).
- Reinhardt, H.F. et al., Sonic Stereometry in Microsurgical Procedures for Deep-Seated Brain Tumors and Vascular Malformations, Neurosurgery, vol. 32, No. 1, pp. 51-57 (Jan. 1993).
- Reinhardt, H.F., et al., Mikrochirurgische Entfernung tiefliegender Gefäßmißbildungen mit Hilfe der Sonar-Stereometrie (Microsurgical Removal of Deep-Seated Vascular Malformations Using Sonar Stereometry). Ultraschall in Med. 12, pp. 80-83 (1991).
- Reinhardt, Hans. F., Neuronavigation: A Ten-Year Review, Neurosurgery, pp. 329-341, (1996).
- Roberts et al., "A frameless stereotactic integration of computerized tomographic imaging and the operating microscope," J. Neurosurg., vol. 65, Oct. 1986, pp. 545-549.
- Rosenbaum et al., "Computerized Tomography Guided Stereotaxis: A New Approach," Applied Neurophysiology, vol. 43, No. 3-5, 1980, pp. 172-173.
- Sautot, "Vissage Pediculaire Assiste Par Ordinateur," 4 pages, Sep. 20, 1994.
- Schueler et al., "Correction of Image Intensifier Distortion for Three-Dimensional X-Ray Angiography," SPIE Medical Imaging 1995, vol. 2432, pp. 272-279.
- Selvik et al., "A Roentgen Stereophotogrammetric System," Acta Radiologica Diagnosis, 1983, pp. 343-352.
- Shelden et al., "Development of a computerized microstereotactic method for localization and removal of minute CNS lesions under direct 3-D vision," J. Neurosurg., vol. 52, 1980, pp. 21-27.
- Simon, D.A., Accuracy Validation in Image-Guided Orthopaedic Surgery, Second Annual Intl. Symp. on Med. Rob. and Comp-Assisted surgery, MRCAS 1995, pp. 185-192.
- Smith et al., "Computer Methods for Improved Diagnostic Image Display Applied to Stereotactic Neurosurgery," Automedical, vol. 14, 1992, pp. 371-382 (4 unnumbered pages).
- Smith et al., "The Neurostation.TM.—A Highly Accurate, Minimally Invasive Solution to Frameless Stereotactic Neurosurgery," Computerized Medical Imaging and Graphics, vol. 18, Jul.-Aug. 1994, pp. 247-256.
- Smith, K.R., et al. Multimodality Image Analysis and Display Methods for Improved Tumor Localization in Stereotactic Neurosurgery, Annul Intl. Conf. of the IEEE Eng. in Med. and Biol. Soc., vol. 13, No. 1, p. 210 (1991).
- Tan, K., Ph.D., et al., A frameless stereotactic approach to neurosurgical planning based on retrospective patient-image registration, J Neurosurg, vol. 79, pp. 296-303 (Aug. 1993).
- The Laitinen Stereotactic System, E2-E6, undated.
- Thompson, et al., A System for Anatomical and Functional Mapping of the Human Thalamus, Computers and Biomedical Research, vol. 10, pp. 9-24 (1977).
- Trobraugh, J.W., et al., Frameless Stereotactic Ultrasonography: Method and Applications, Computerized Medical Imaging and Graphics, vol. 18, No. 4, pp. 235-246 (1994).
- Viant et al., "A Computer Assisted Orthopaedic System for Distal Locking of Intramedullary Nails," Proc. of MediMEC '95, Bristol, 1995, pp. 86-91.
- Von Hanwhr et al., Foreword, Computerized Medical Imaging and Graphics, vol. 18, No. 4, pp. 225-228, (Jul.-Aug. 1994).
- Wang, M.Y., et al., An Automatic Technique for Finding and Localizing Externally Attached Markers in CT and MR Volume Images of the Head, IEEE Trans. on Biomed. Eng., vol. 43, No. 6, pp. 627-637 (Jun. 1996).
- Watanabe et al., "Three-Dimensional Digitizer (Neuronavigator): New Equipment for Computed Tomography-Guided Stereotactic Surgery," Surgical Neurology, vol. 27, No. 6, Jun. 1987, pp. 543-547.
- Watanabe, E., M.D., et al., Open Surgery Assisted by the Neuronavigator, a Stereotactic, Articulated, Sensitive Arm, Neurosurgery, vol. 28, No. 6, pp. 792-800 (1991).

(56)

References Cited

OTHER PUBLICATIONS

Weese et al., "An Approach to 2D/3D Registration of a Vertebra in 2D X-ray Fluoroscopies with 3D Ct Images," pp. 119-128, undated. Written Opinion dated Aug. 14, 2001 for PCT/US00/29880.

Medtronic METRx System "Surgical Technique" 31 pages, 2009.

Medtronic "Minimal Access Spinal Technologies" METRx System, 22 pages, 2004.

European Office Action dated Oct. 5, 2017 in corresponding European Application No. 11717425.0.

Office Action dated Jan. 2, 2020 in corresponding/related European Application No. 19200422.4.

International Search Report and Written Opinion dated Aug. 8, 2013 for PCT/US2012/022840 claiming benefit of U.S. Appl. No. 13/016,762, filed Jan. 28, 2011.

International Search Report and Written Opinion dated Aug. 8, 2013 for PCT/US2012/022846 claiming benefit of U.S. Appl. No. 13/016,765, filed Jan. 28, 2011.

Extended European Search Report regarding EP 19200422.4, dated Jan. 1, 2020.

Office Action dated Nov. 17, 2020, in corresponding European Application No. 19200422.4.

Office Action regarding European Application No. 19200422.4, dated Aug. 12, 2021.

* cited by examiner

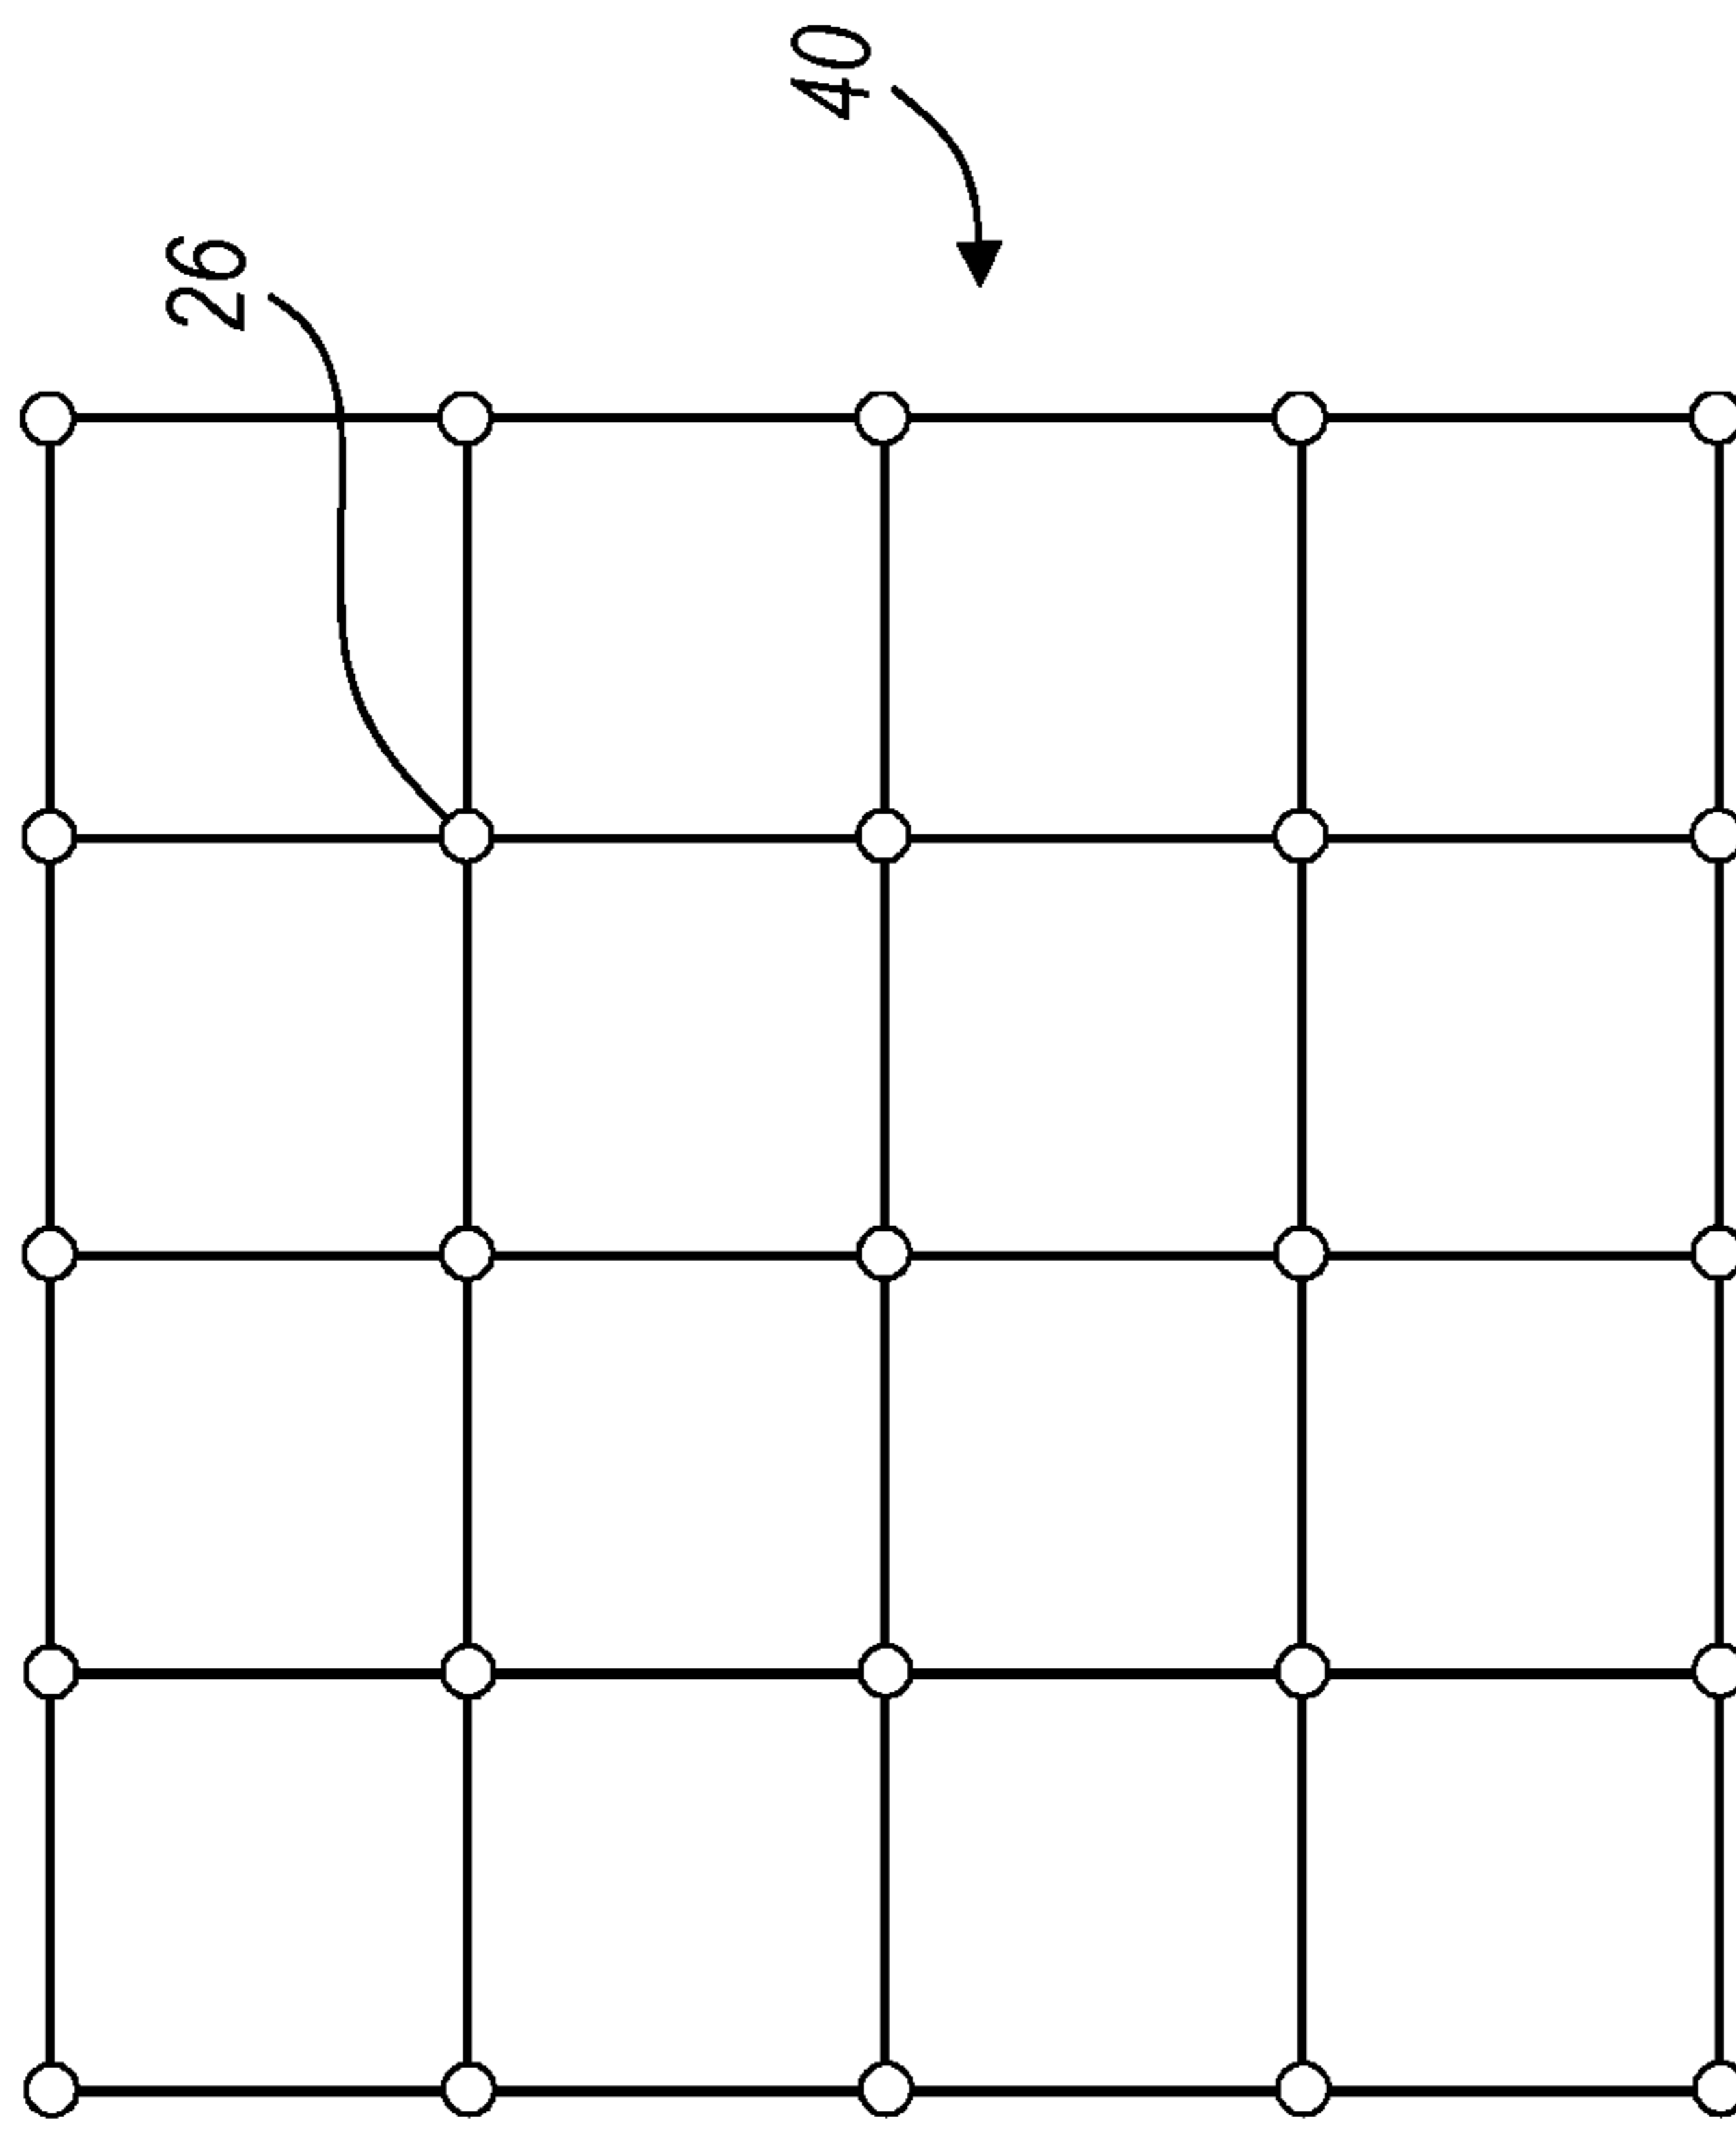
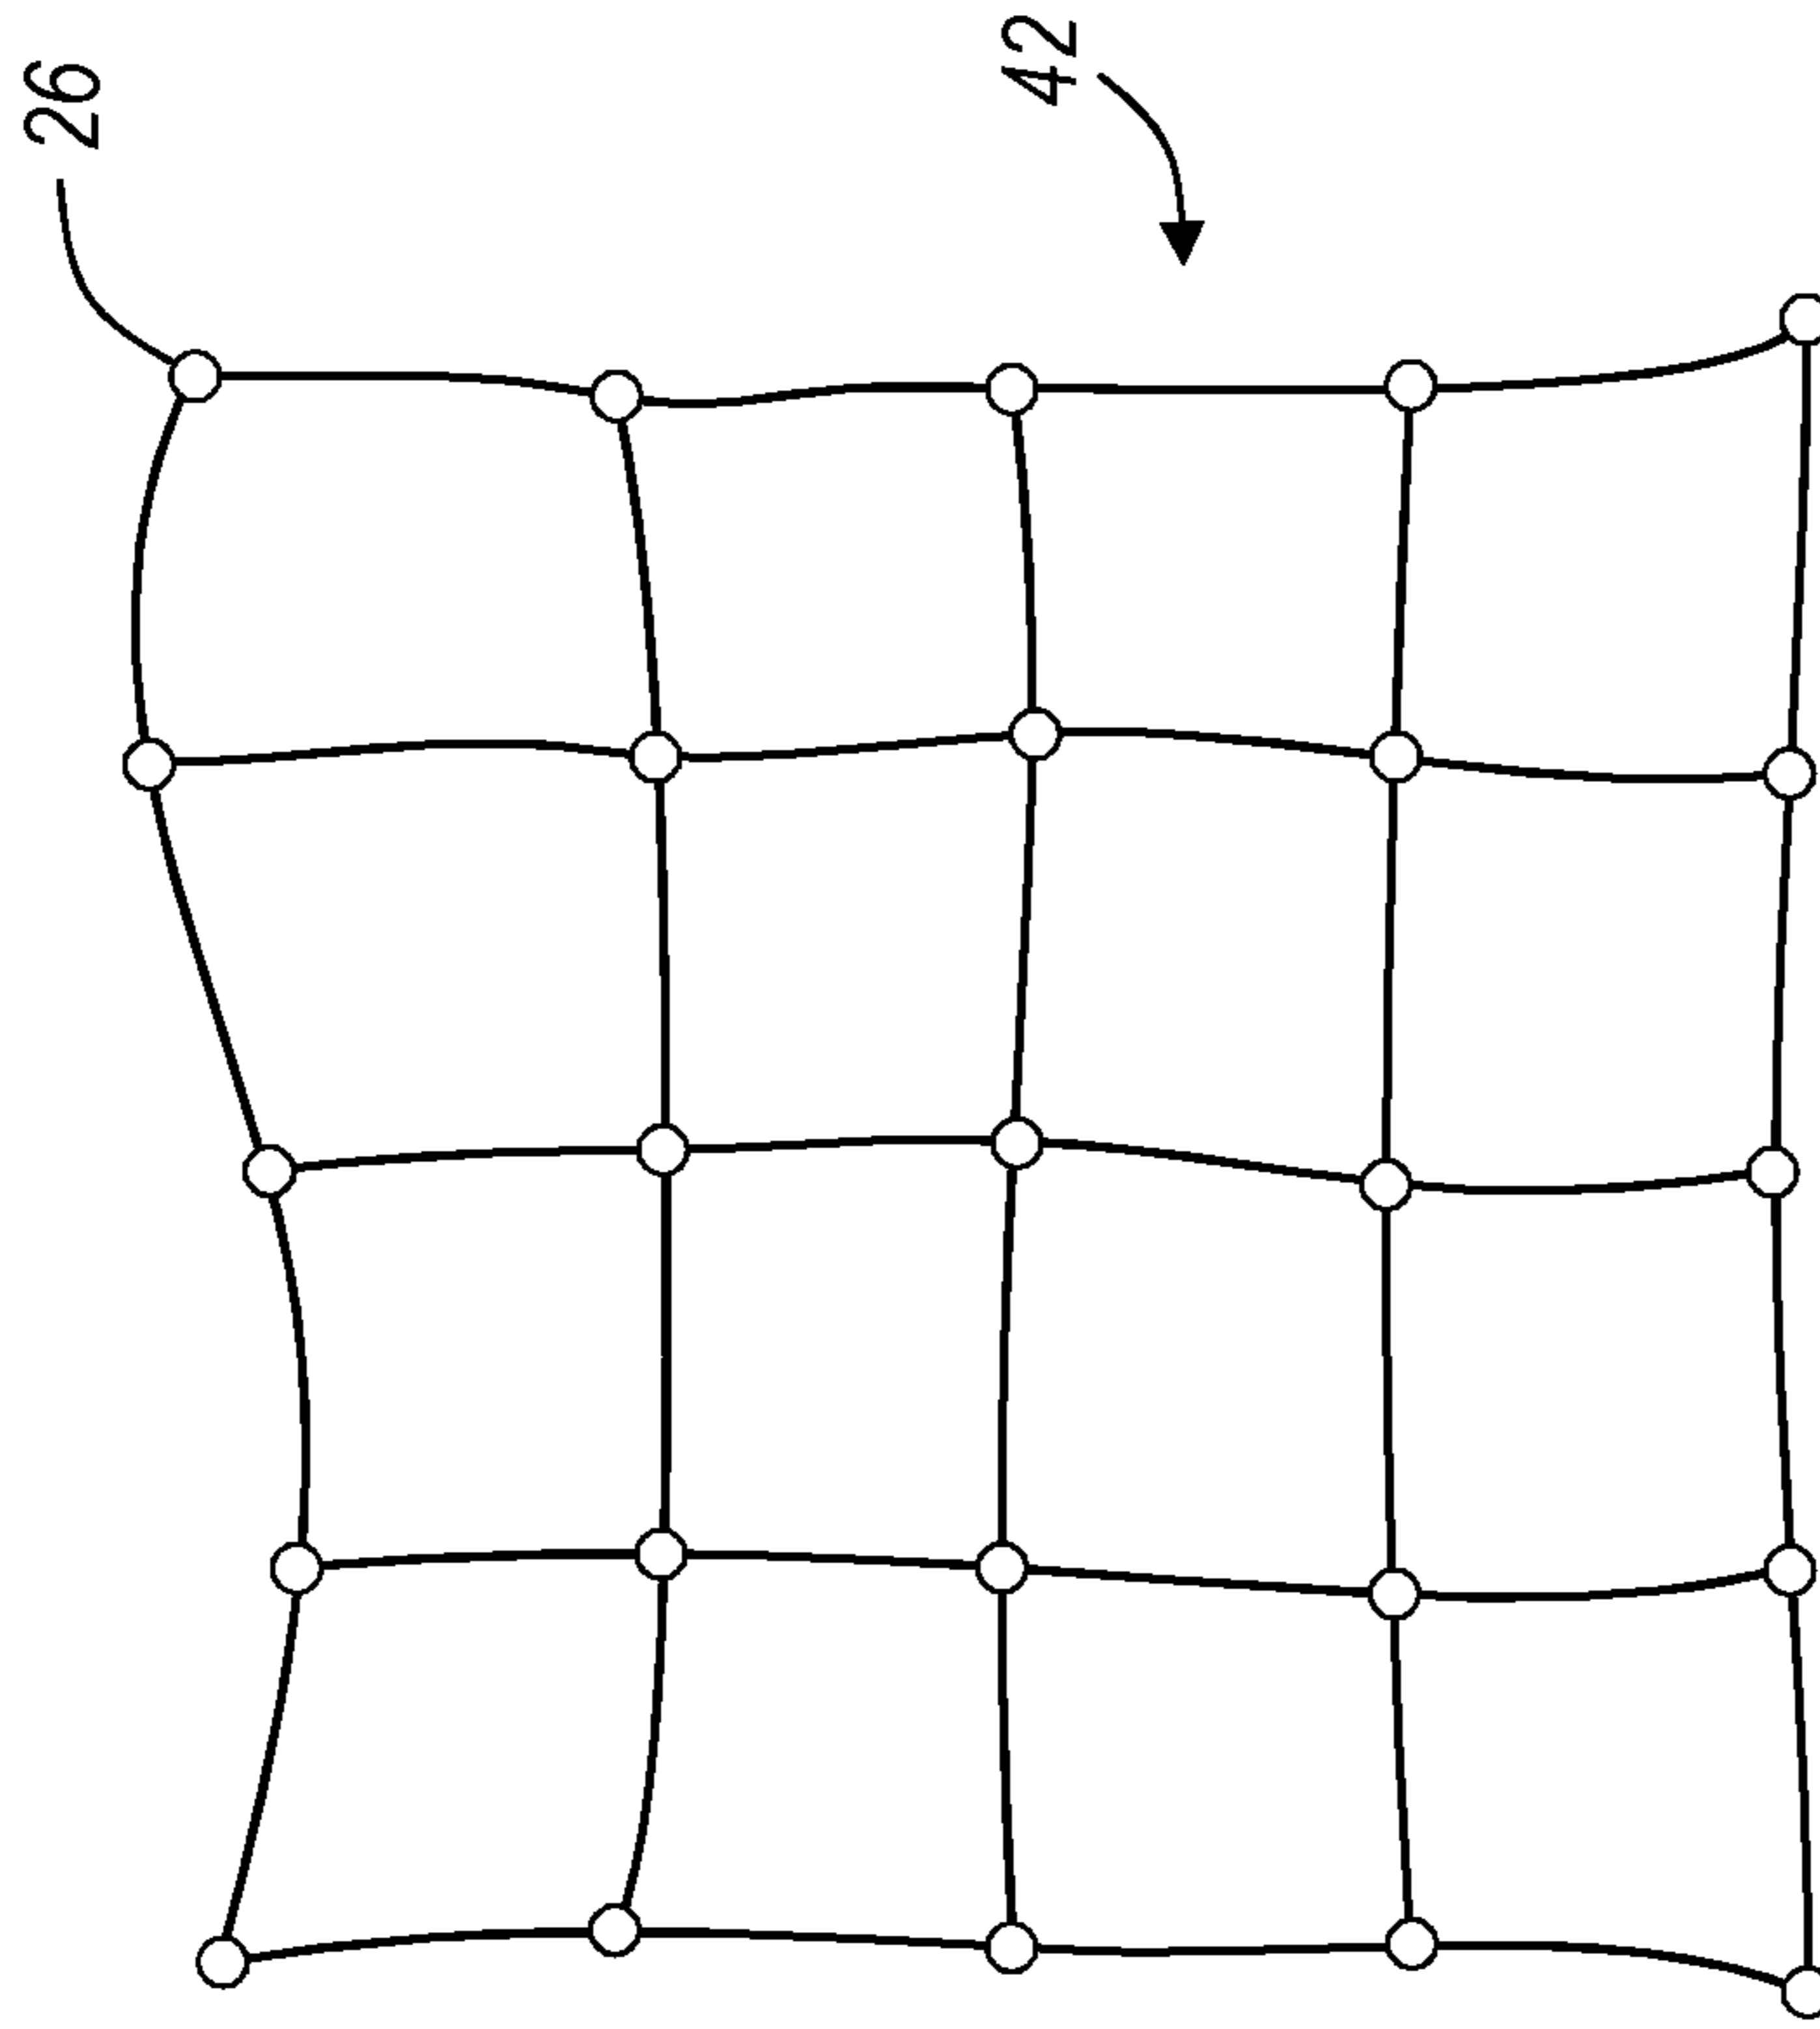


FIG. 2B

FIG. 2A

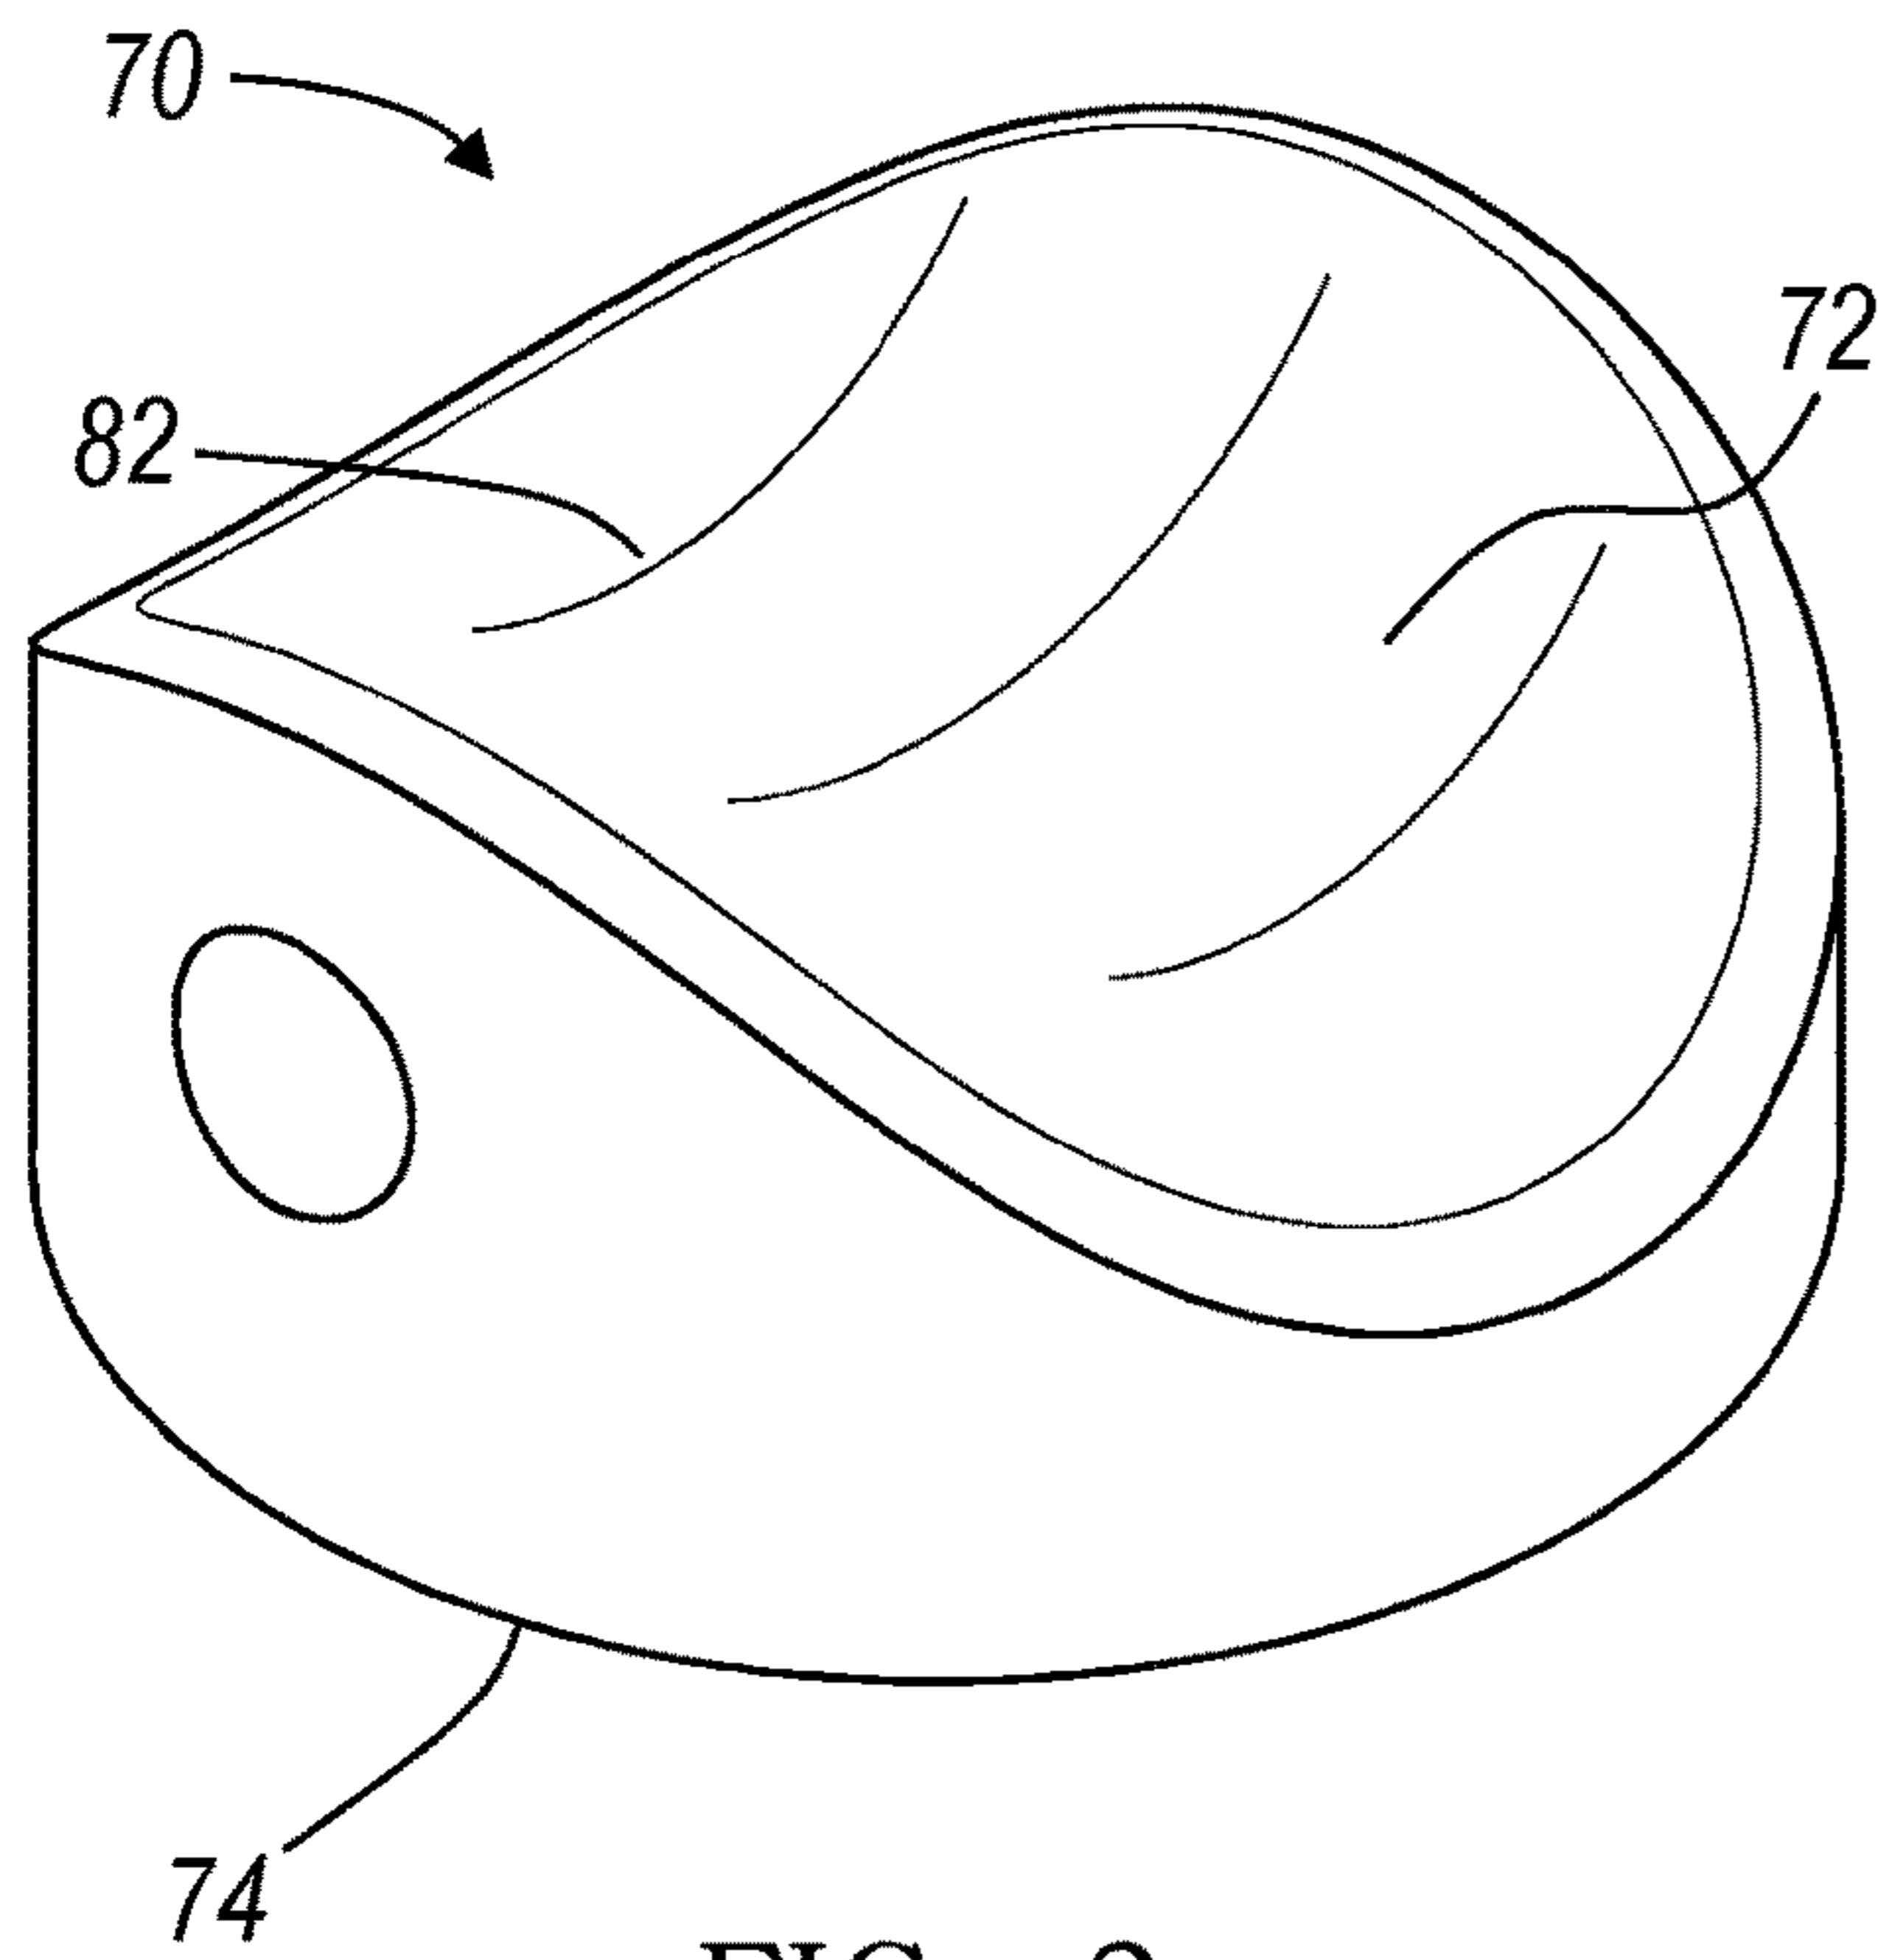


FIG. 3

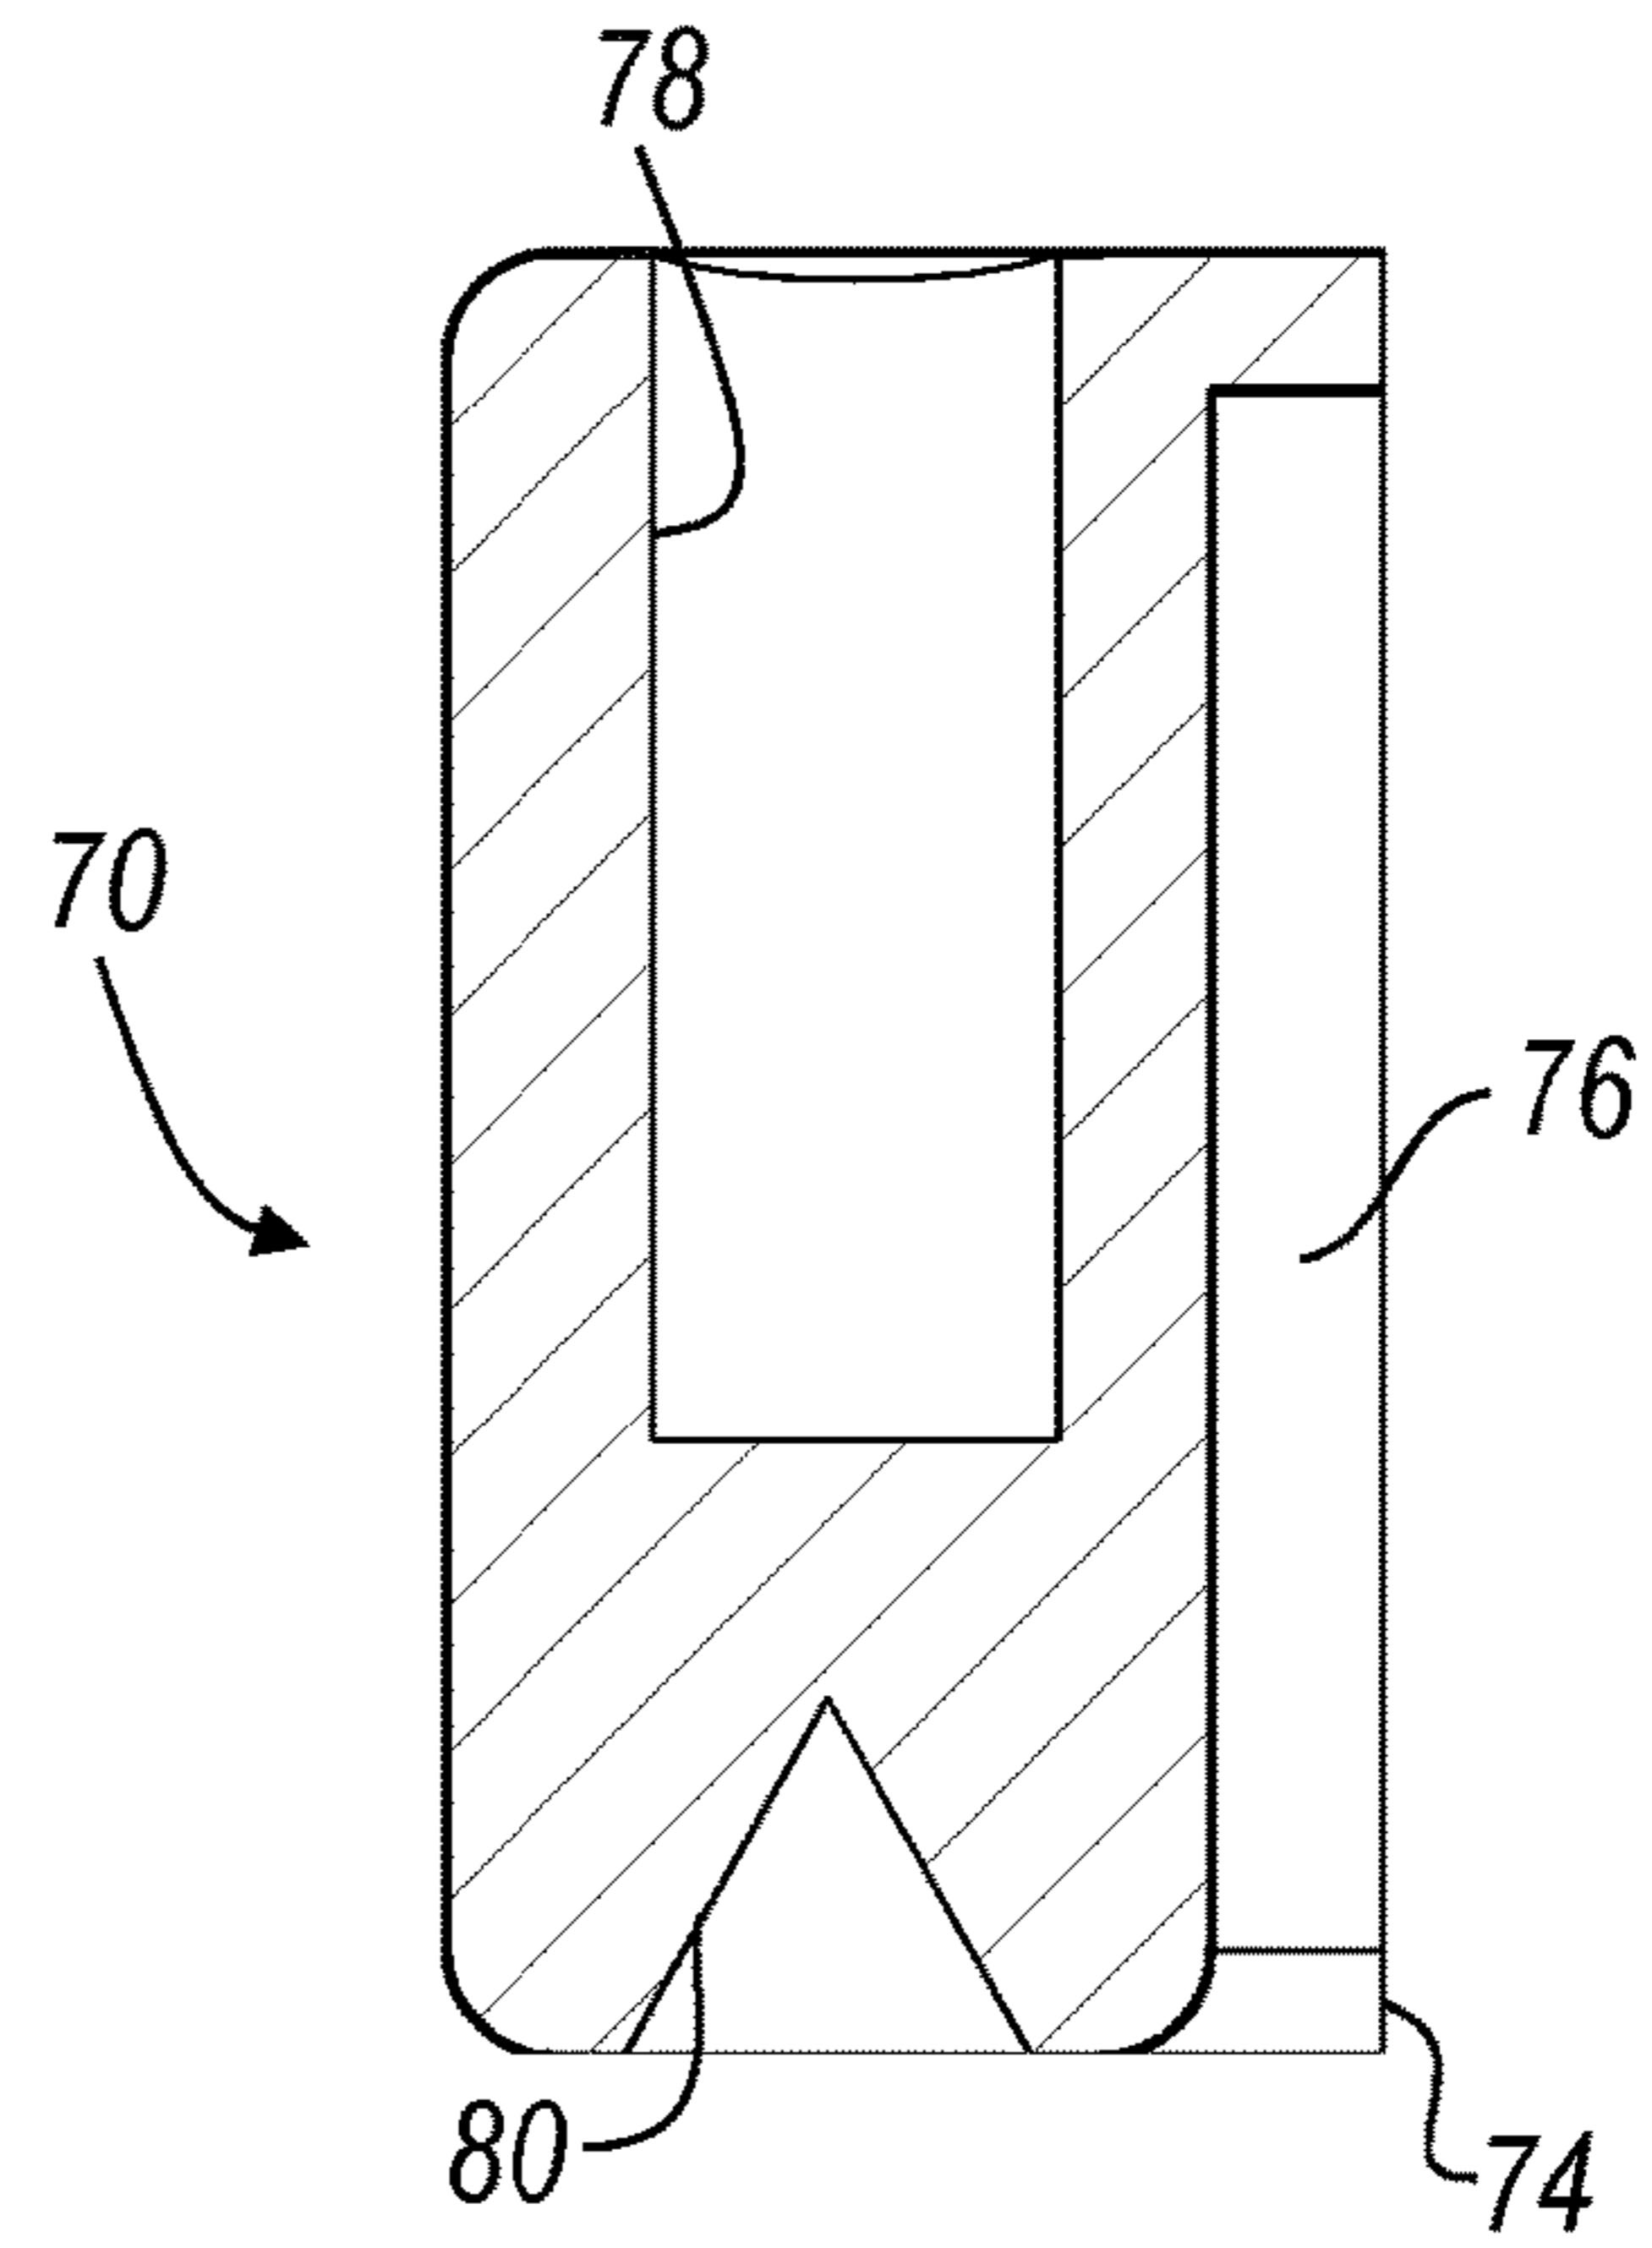


FIG. 4

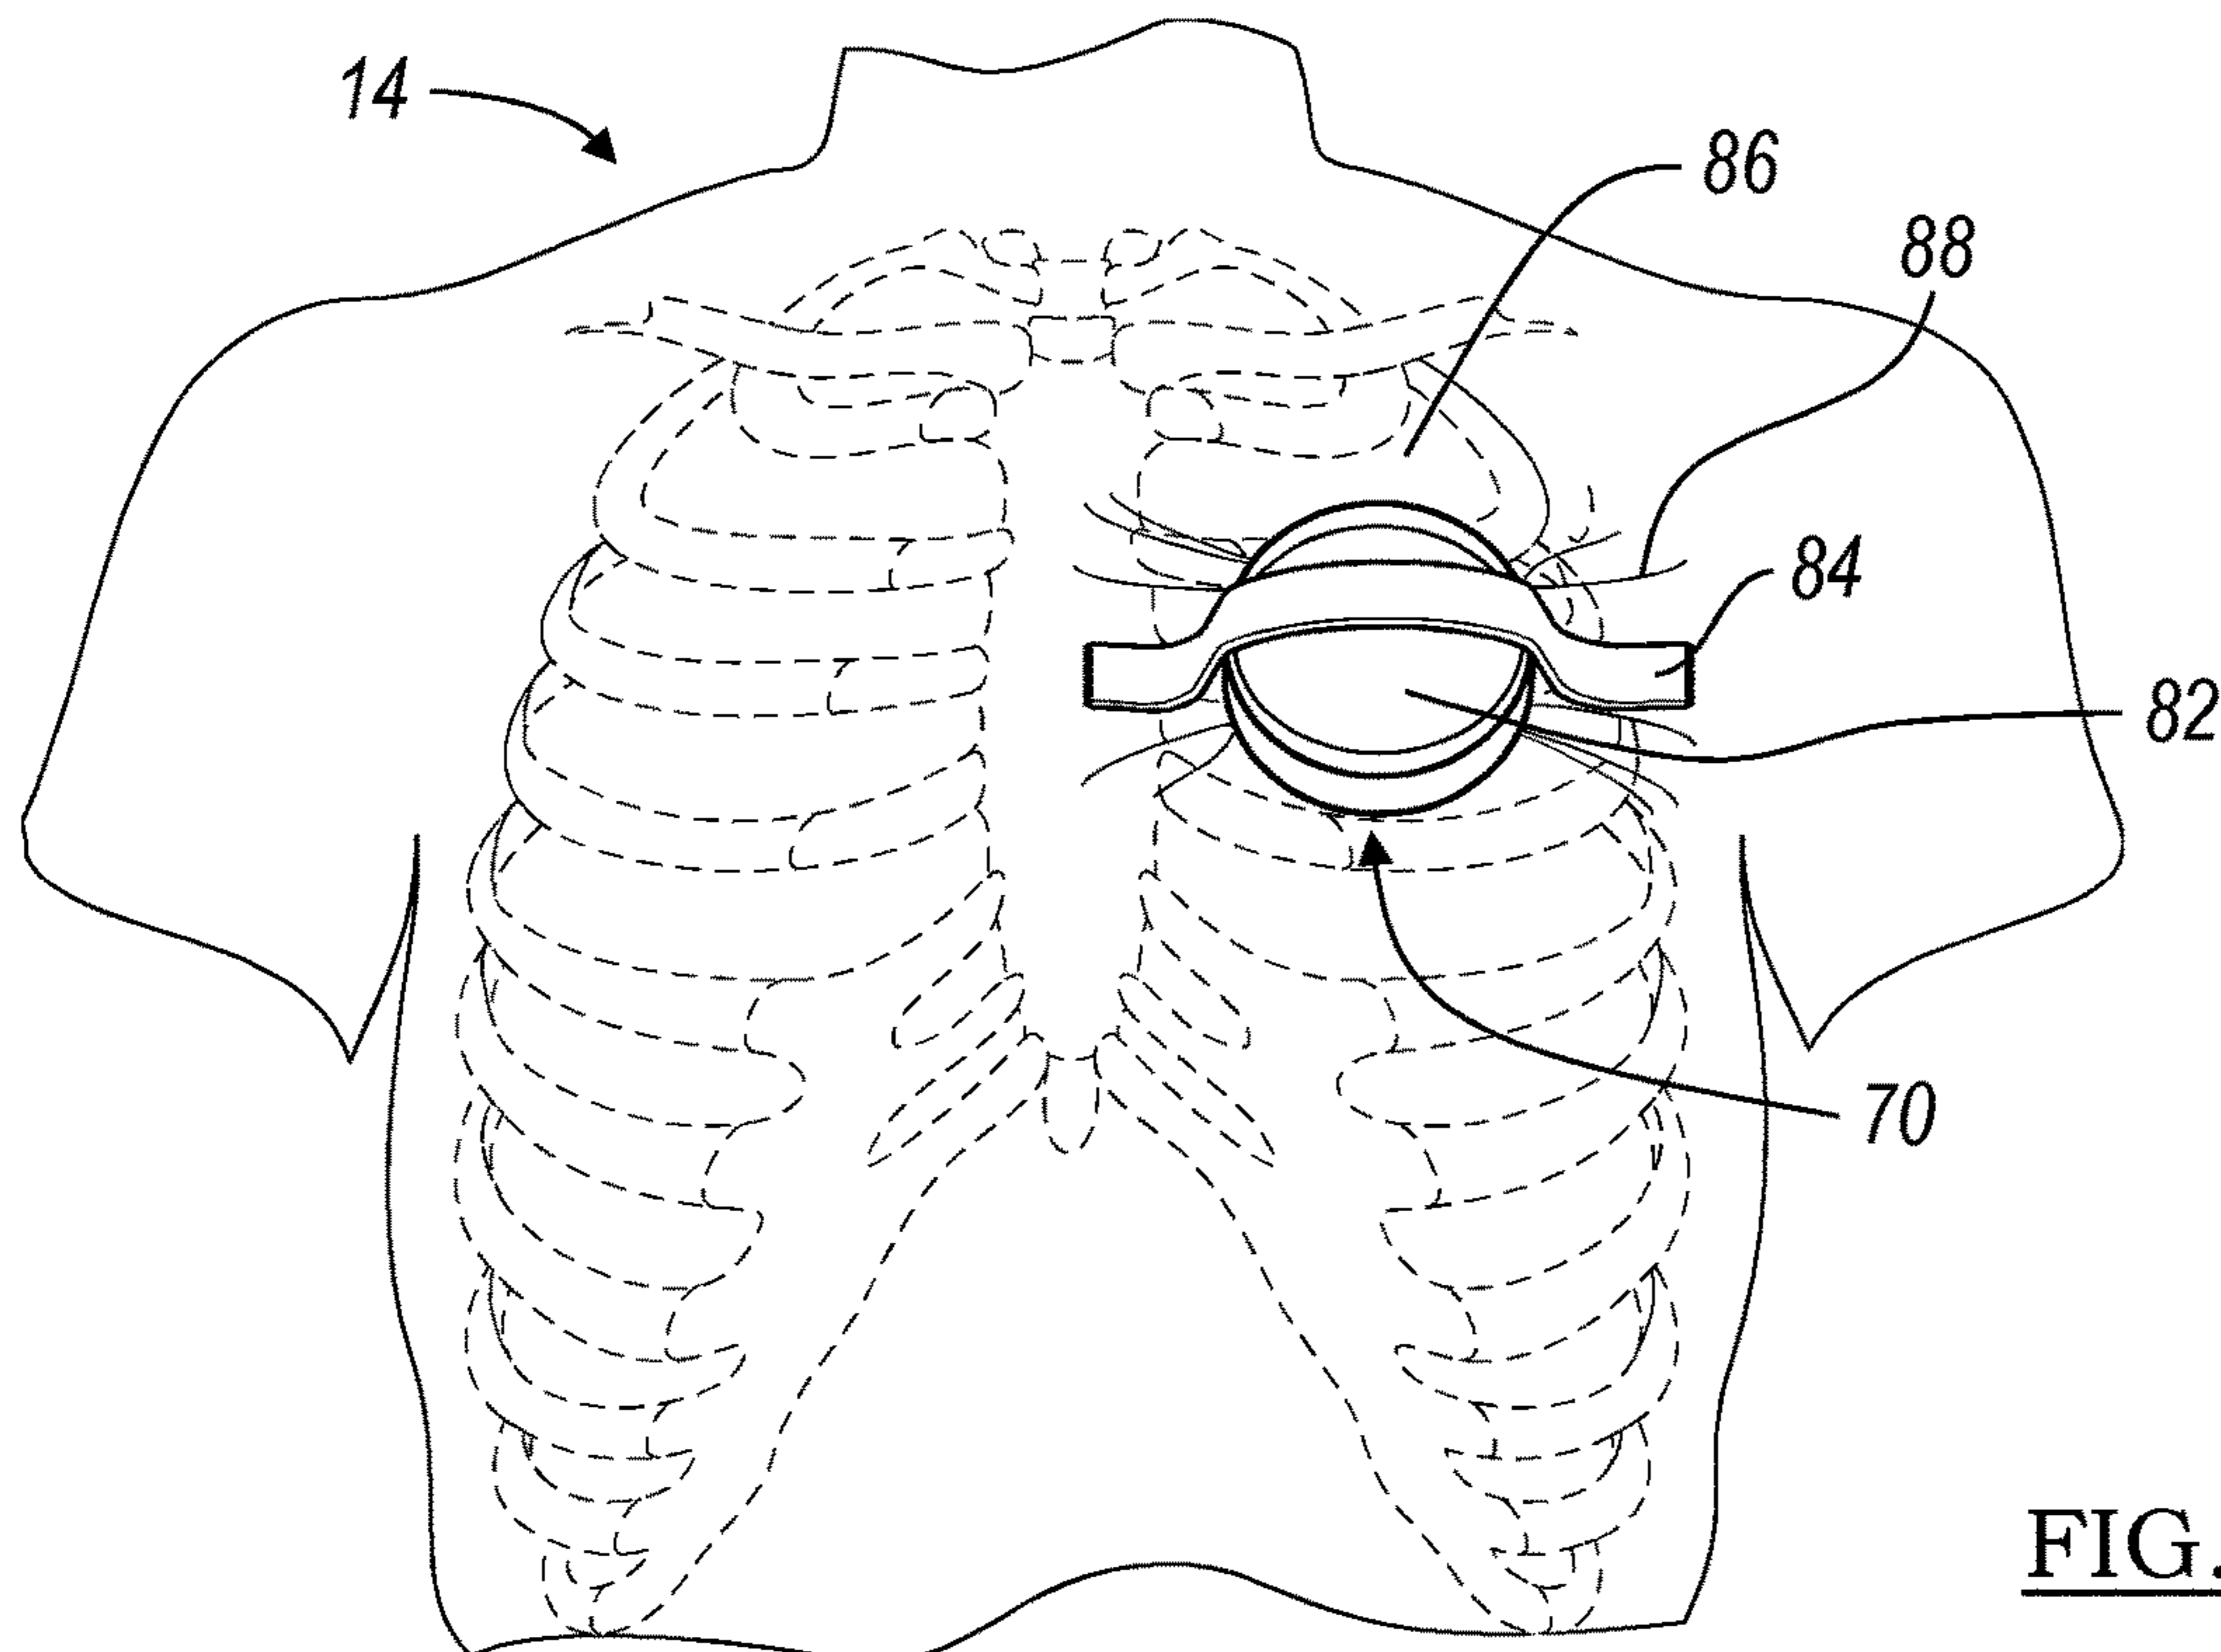


FIG. 5

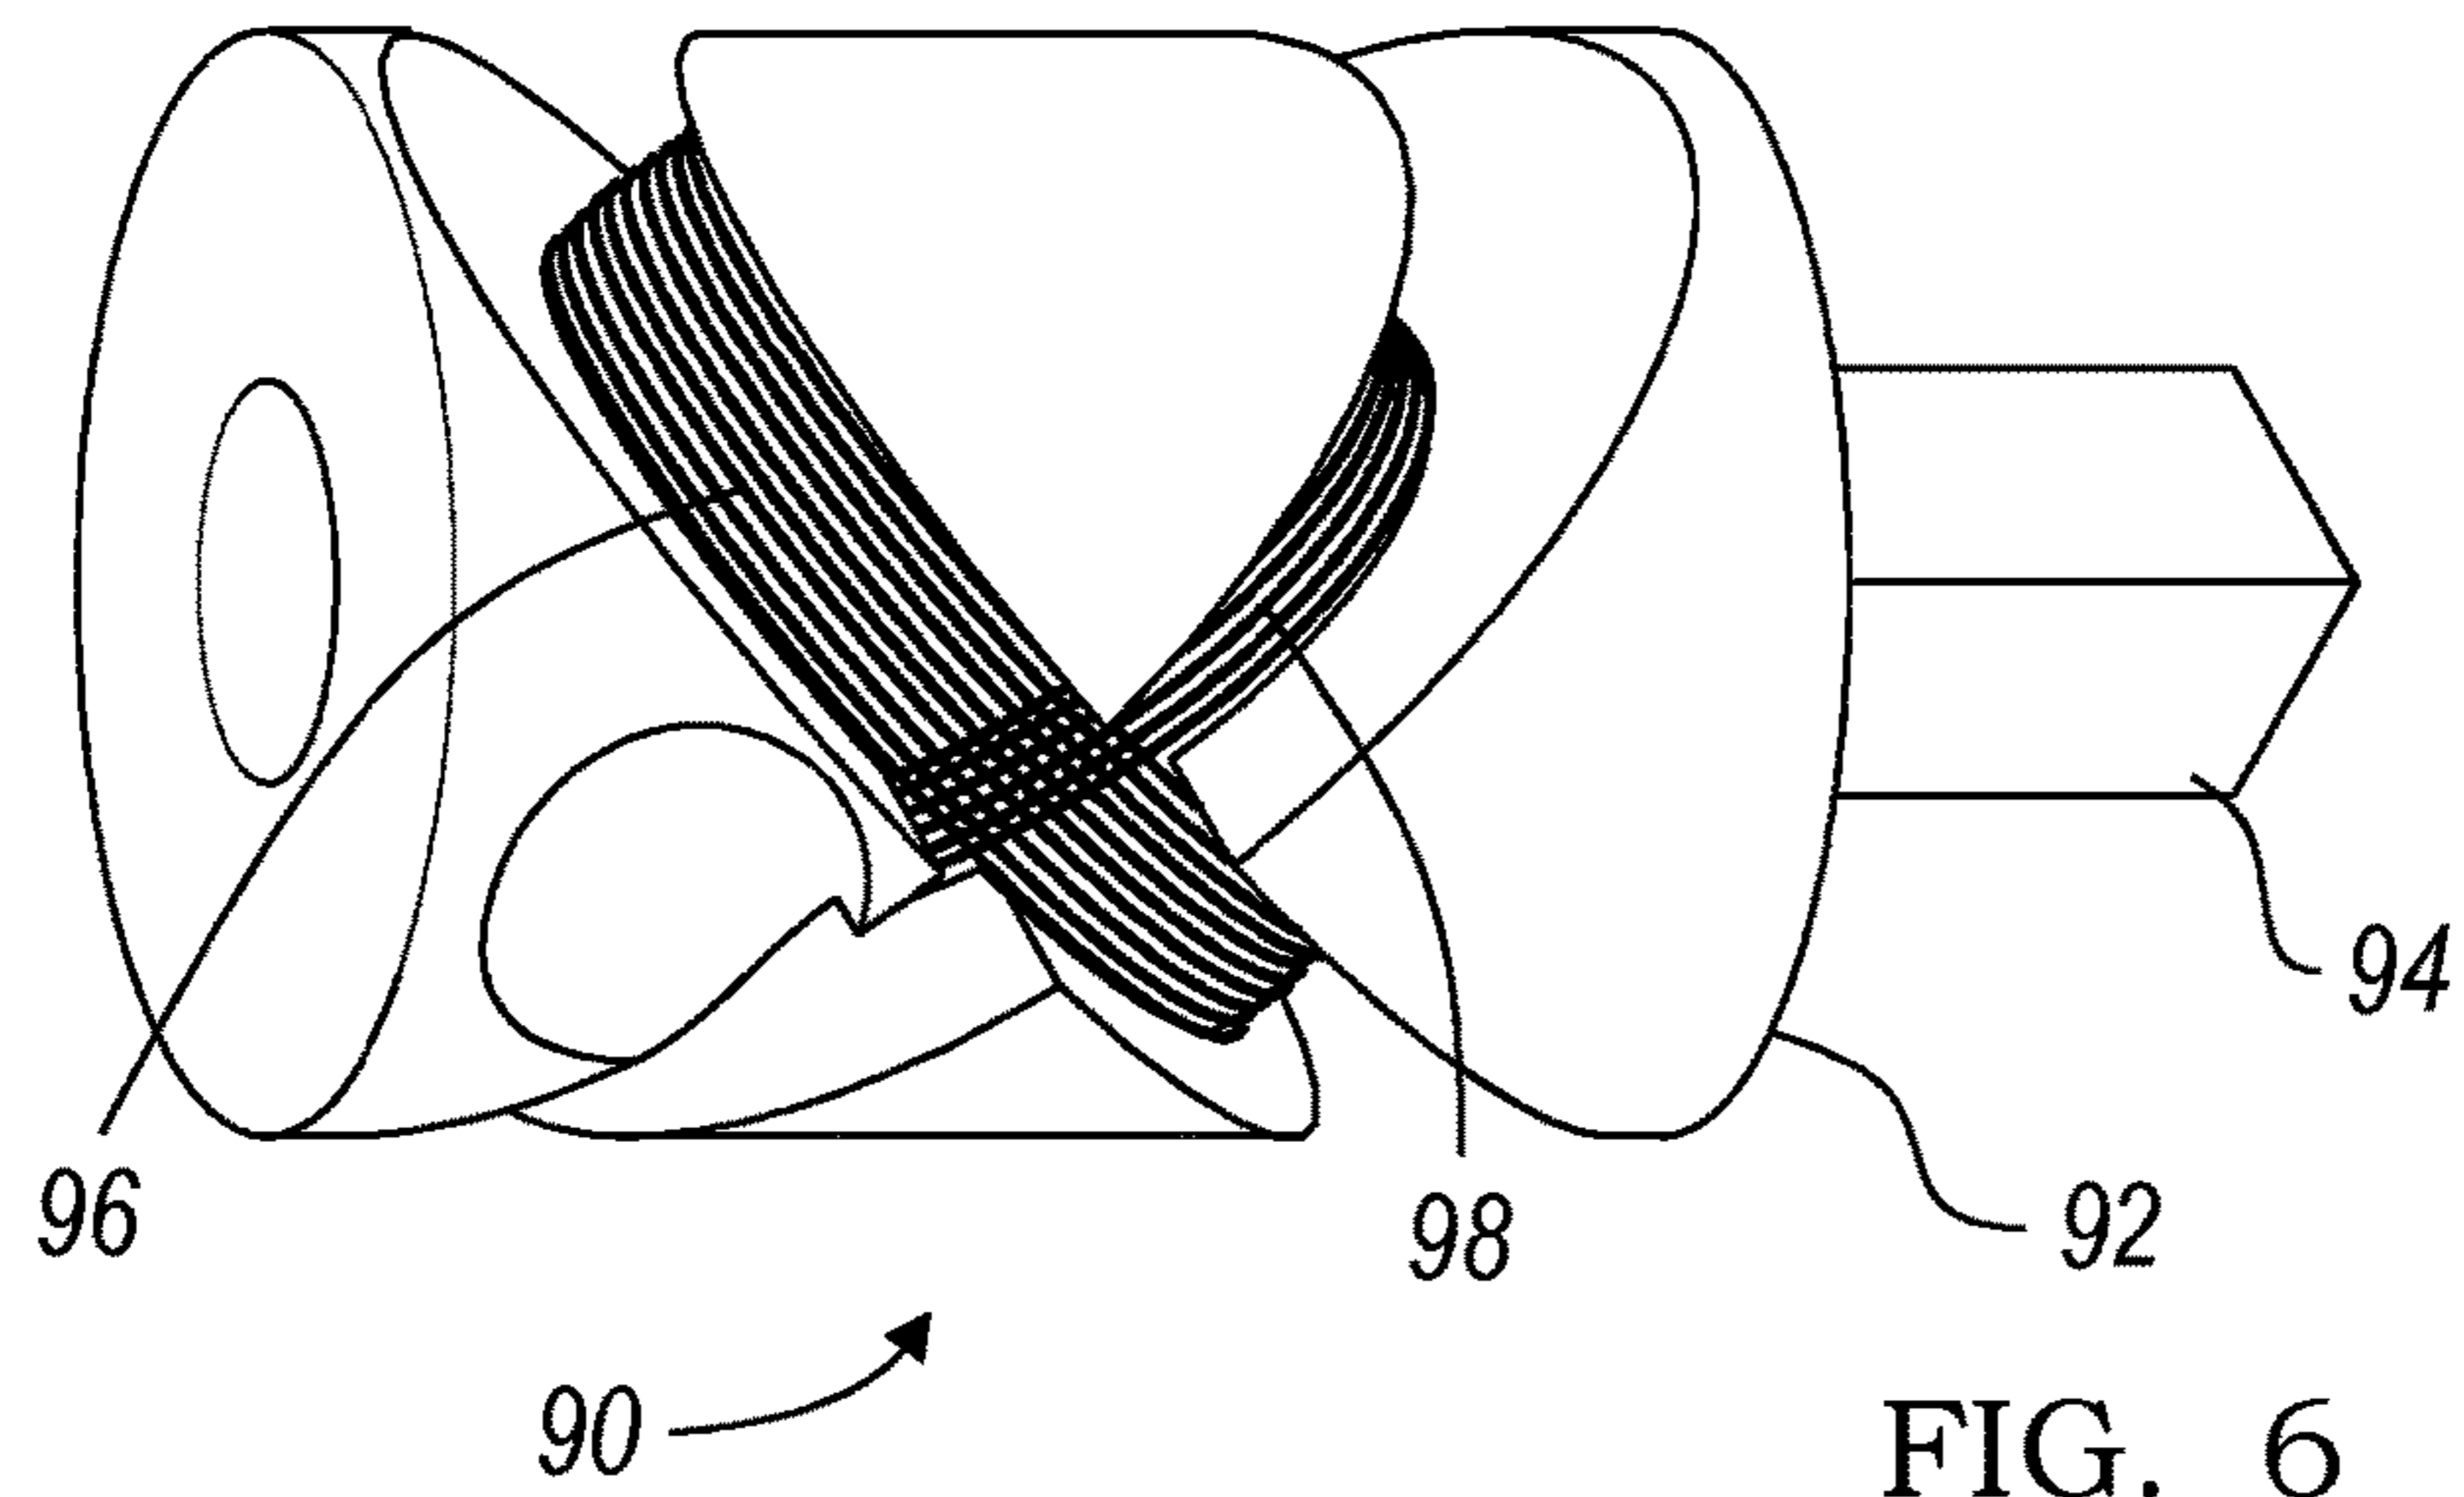


FIG. 6

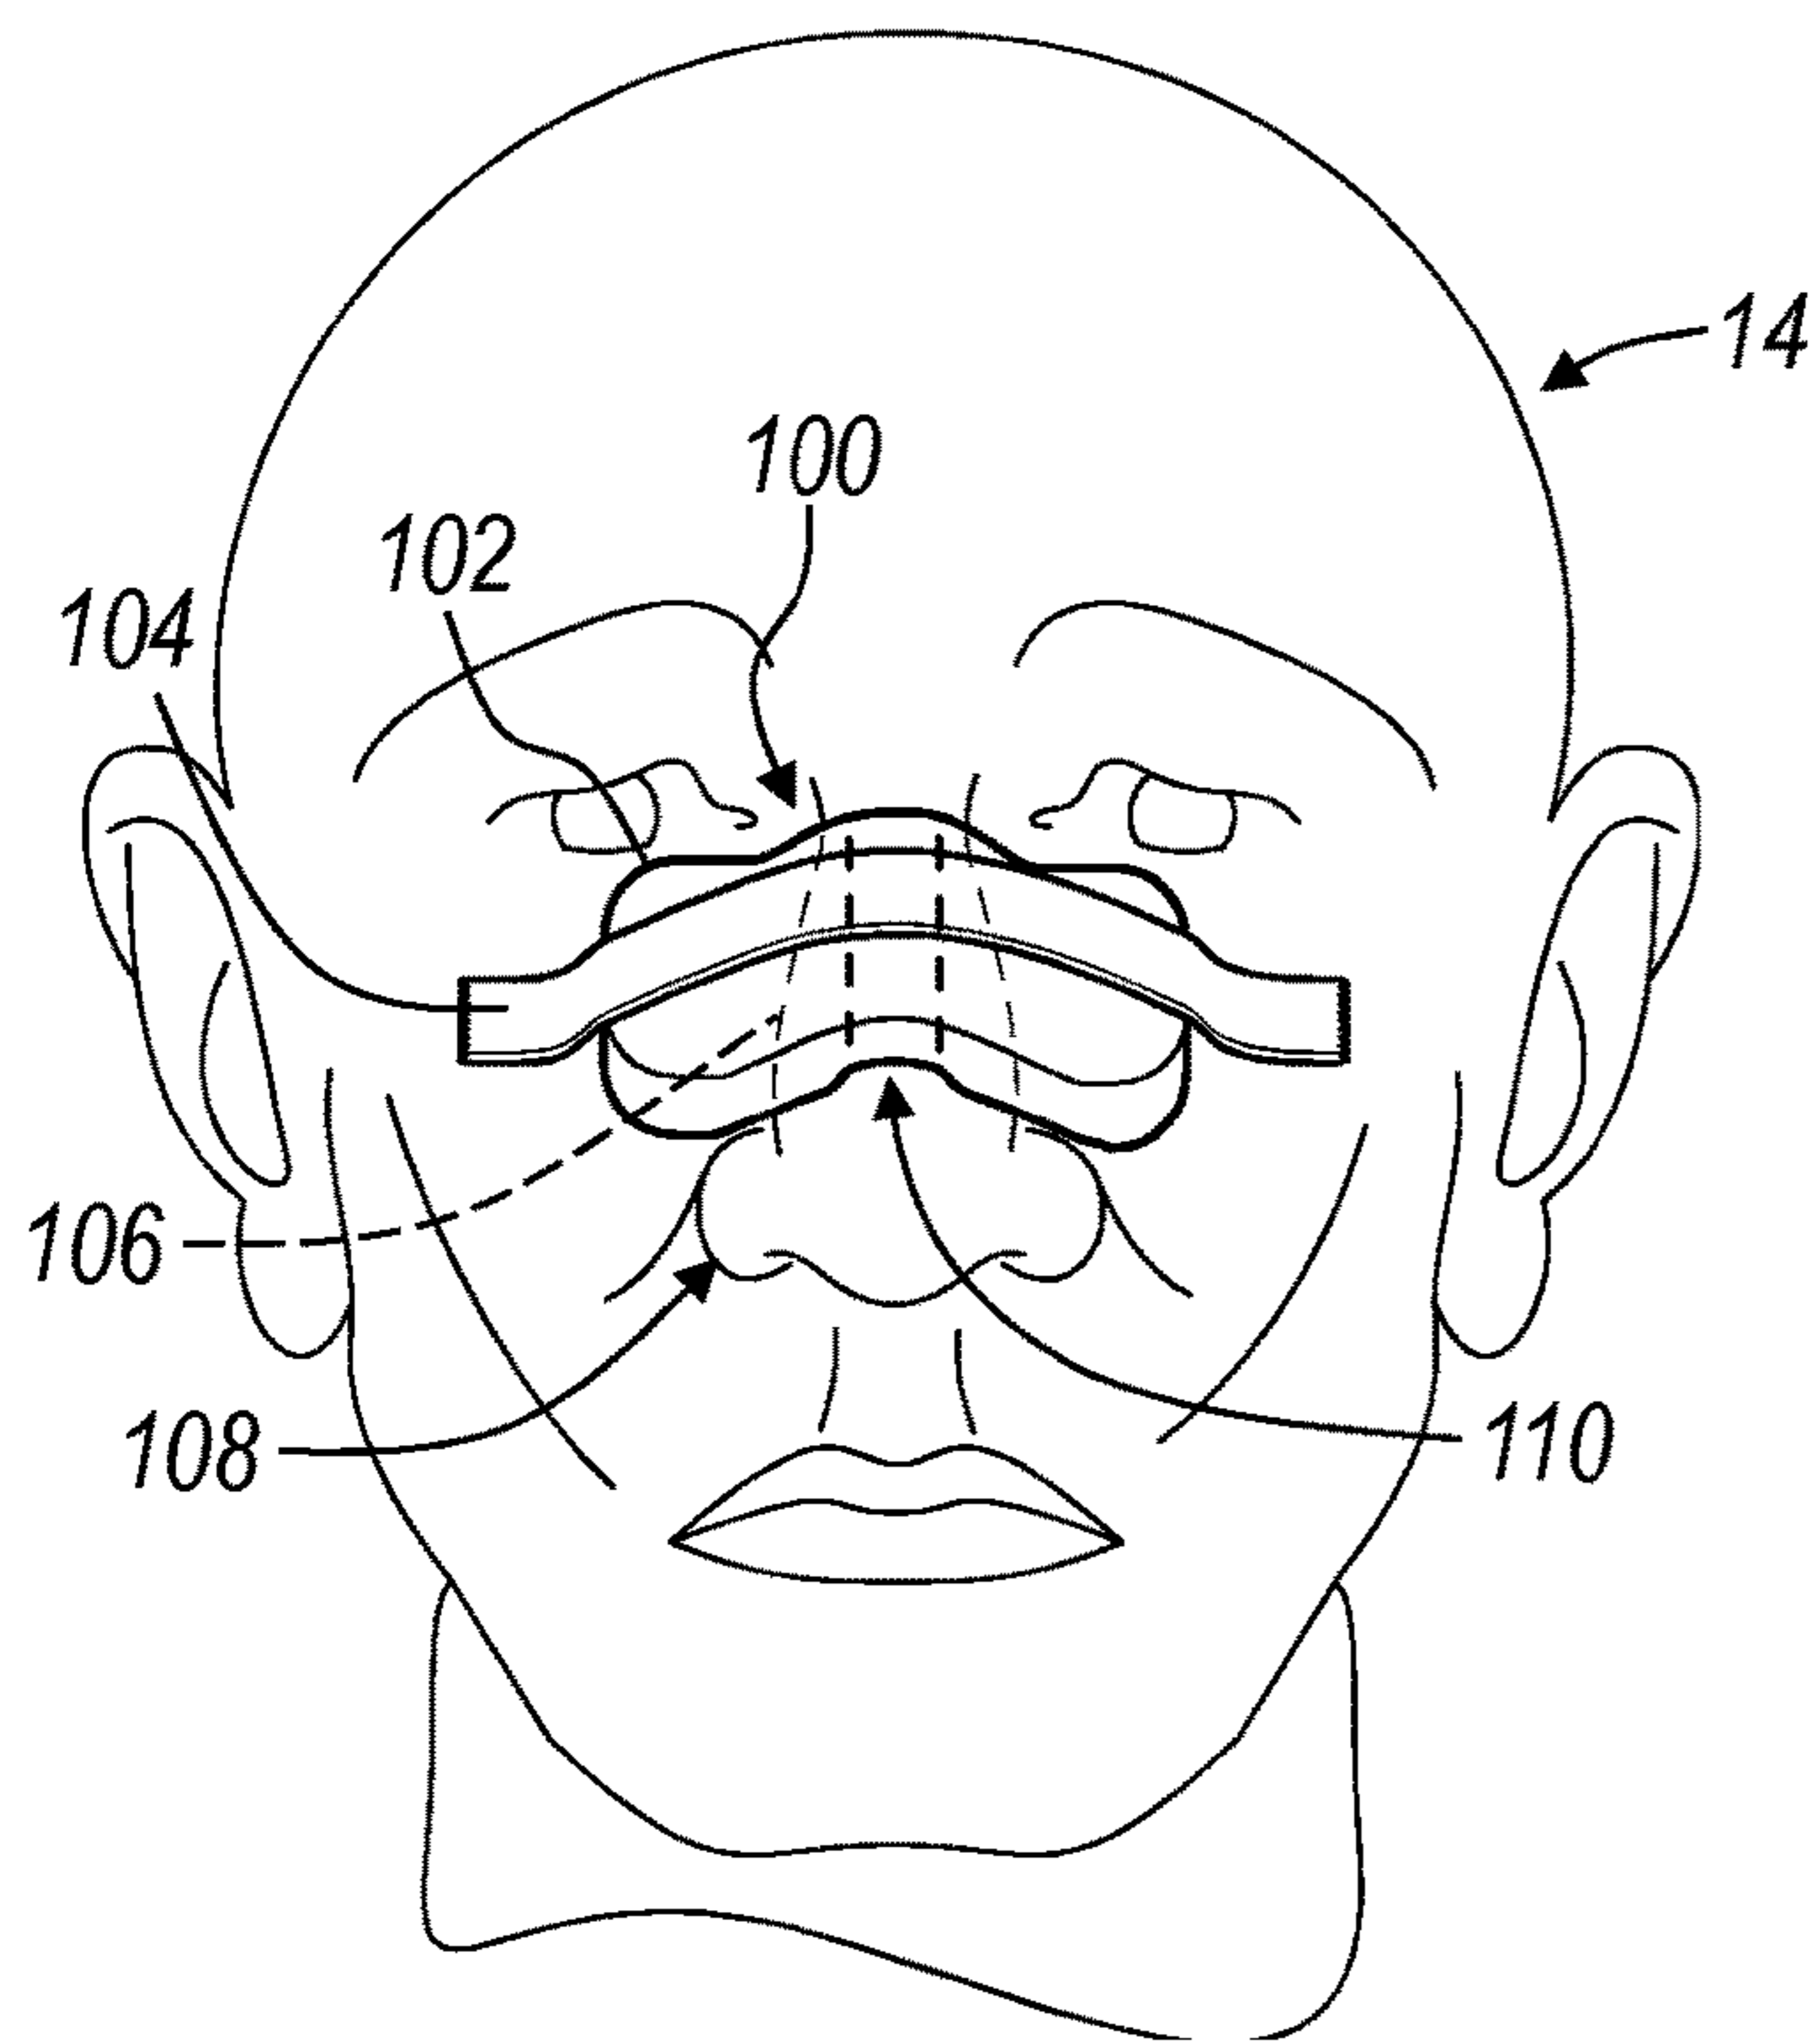


FIG. 7

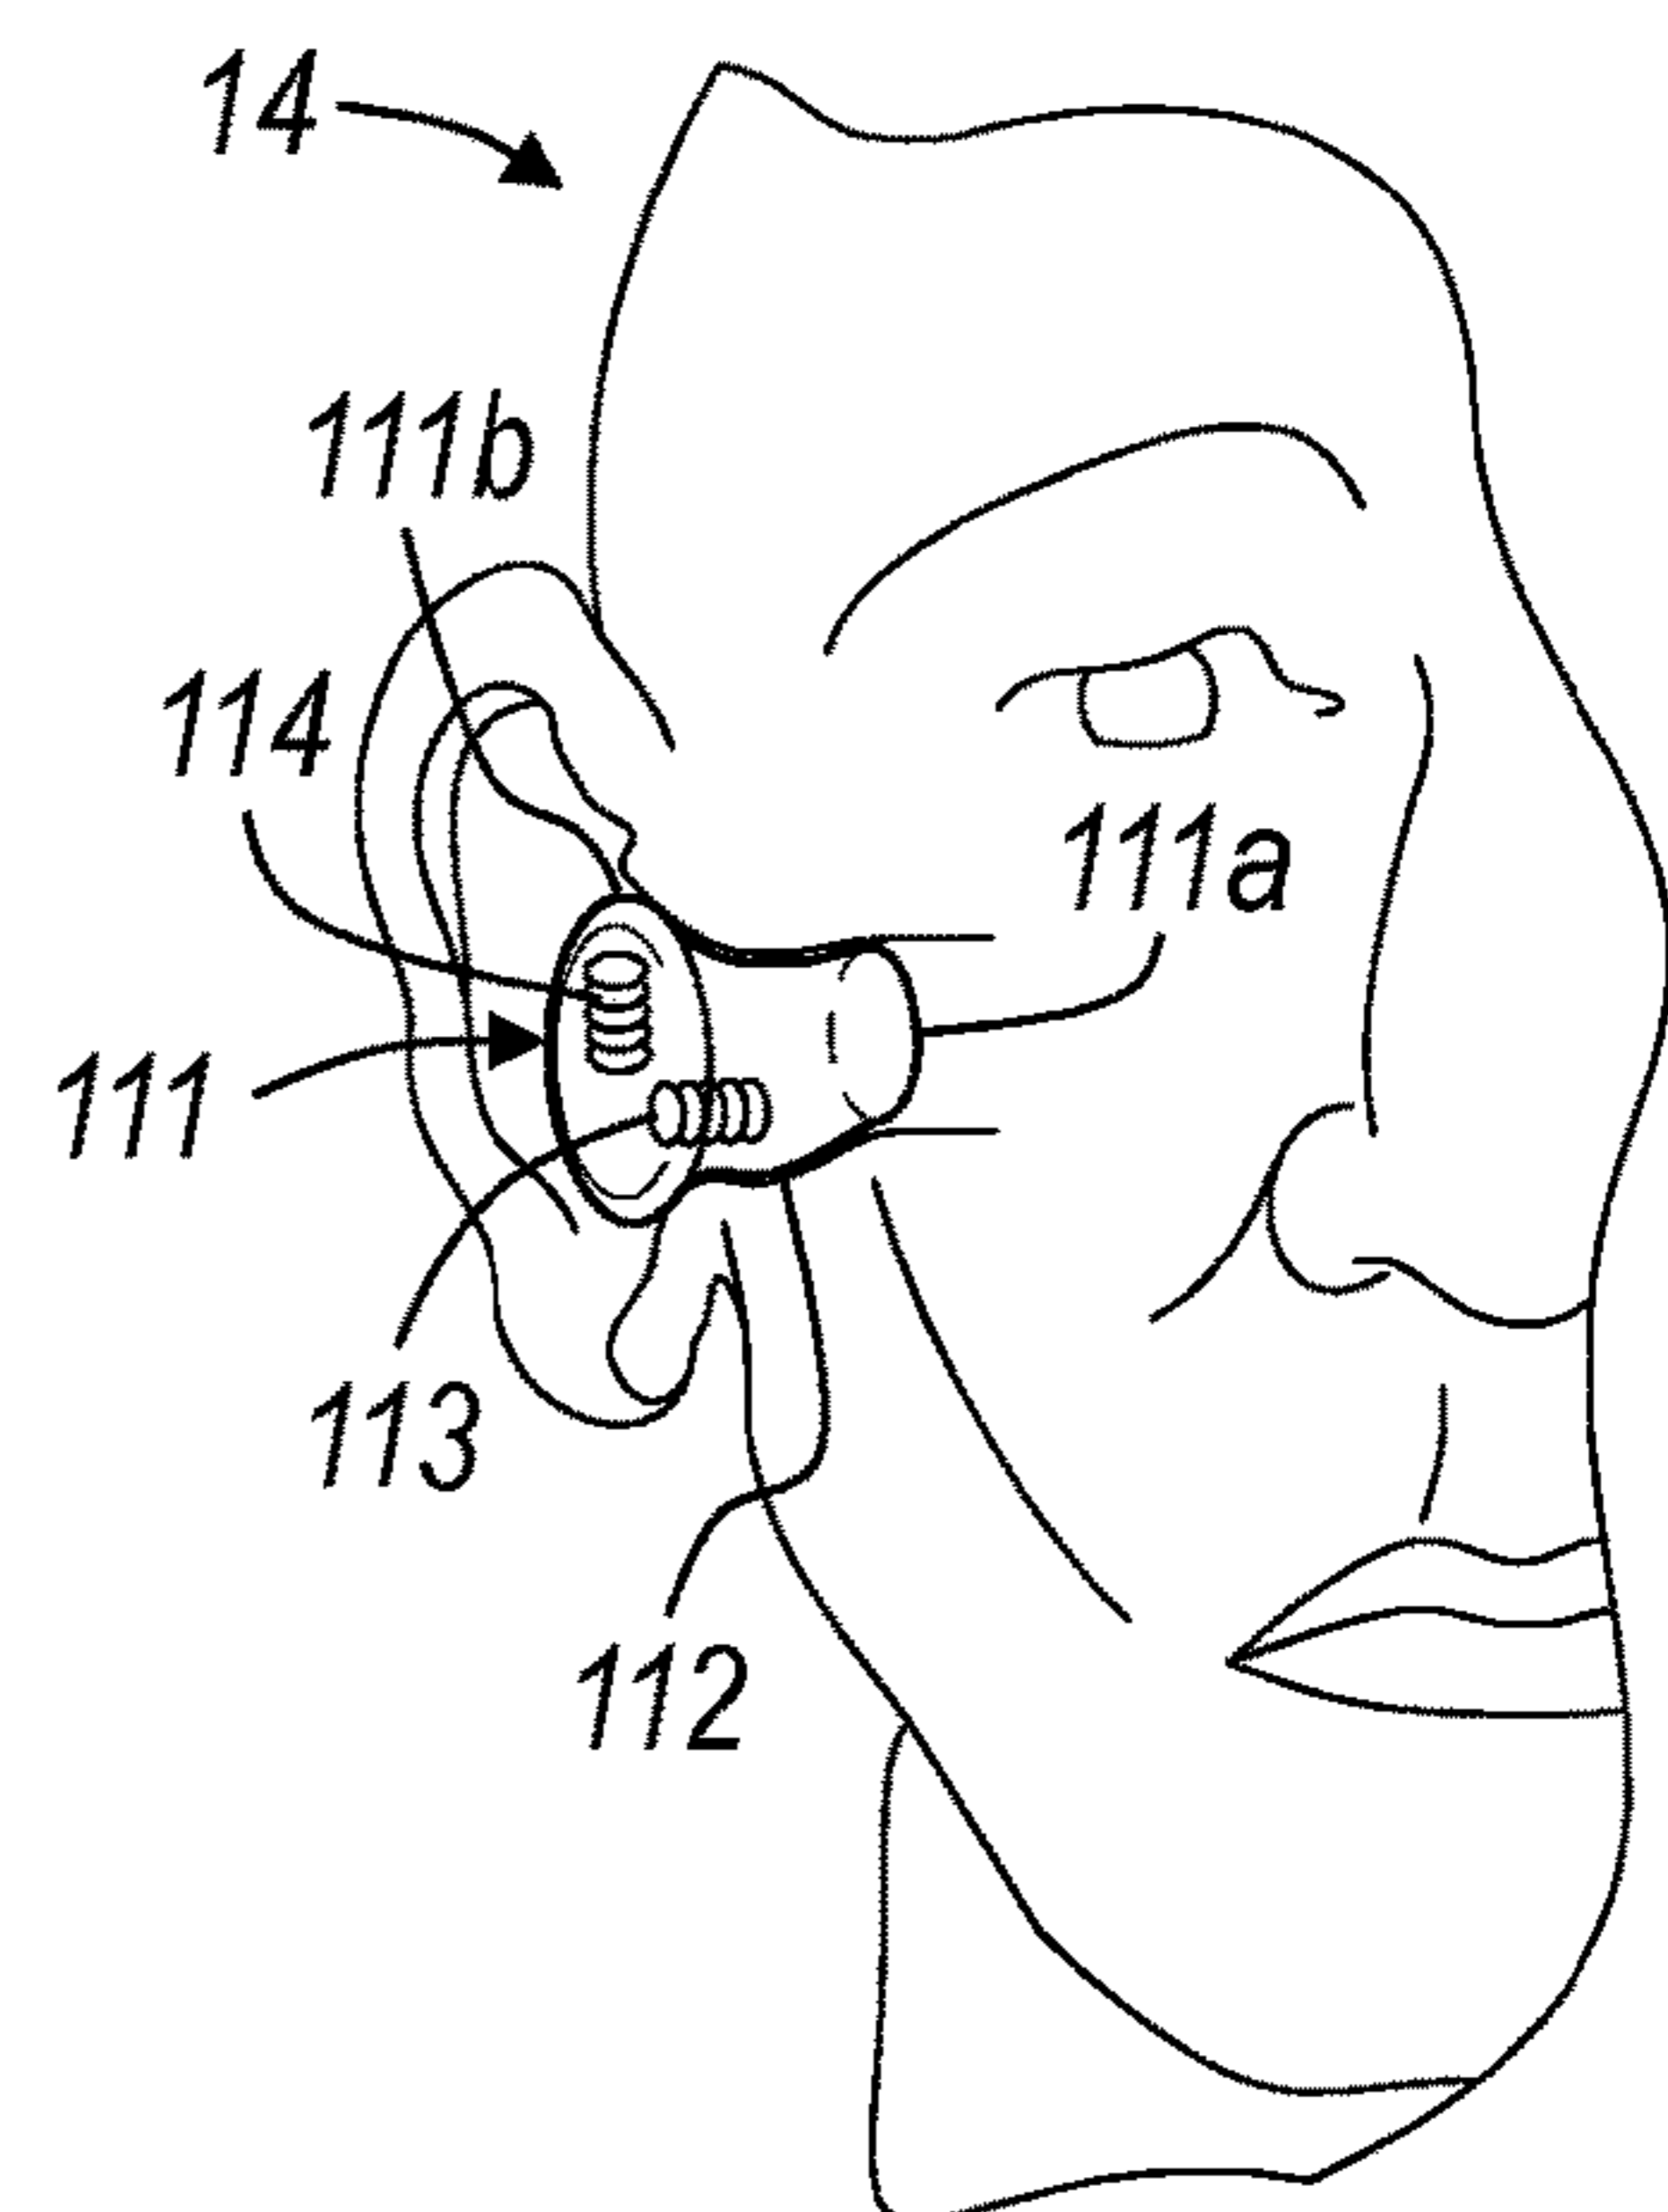


FIG. 8

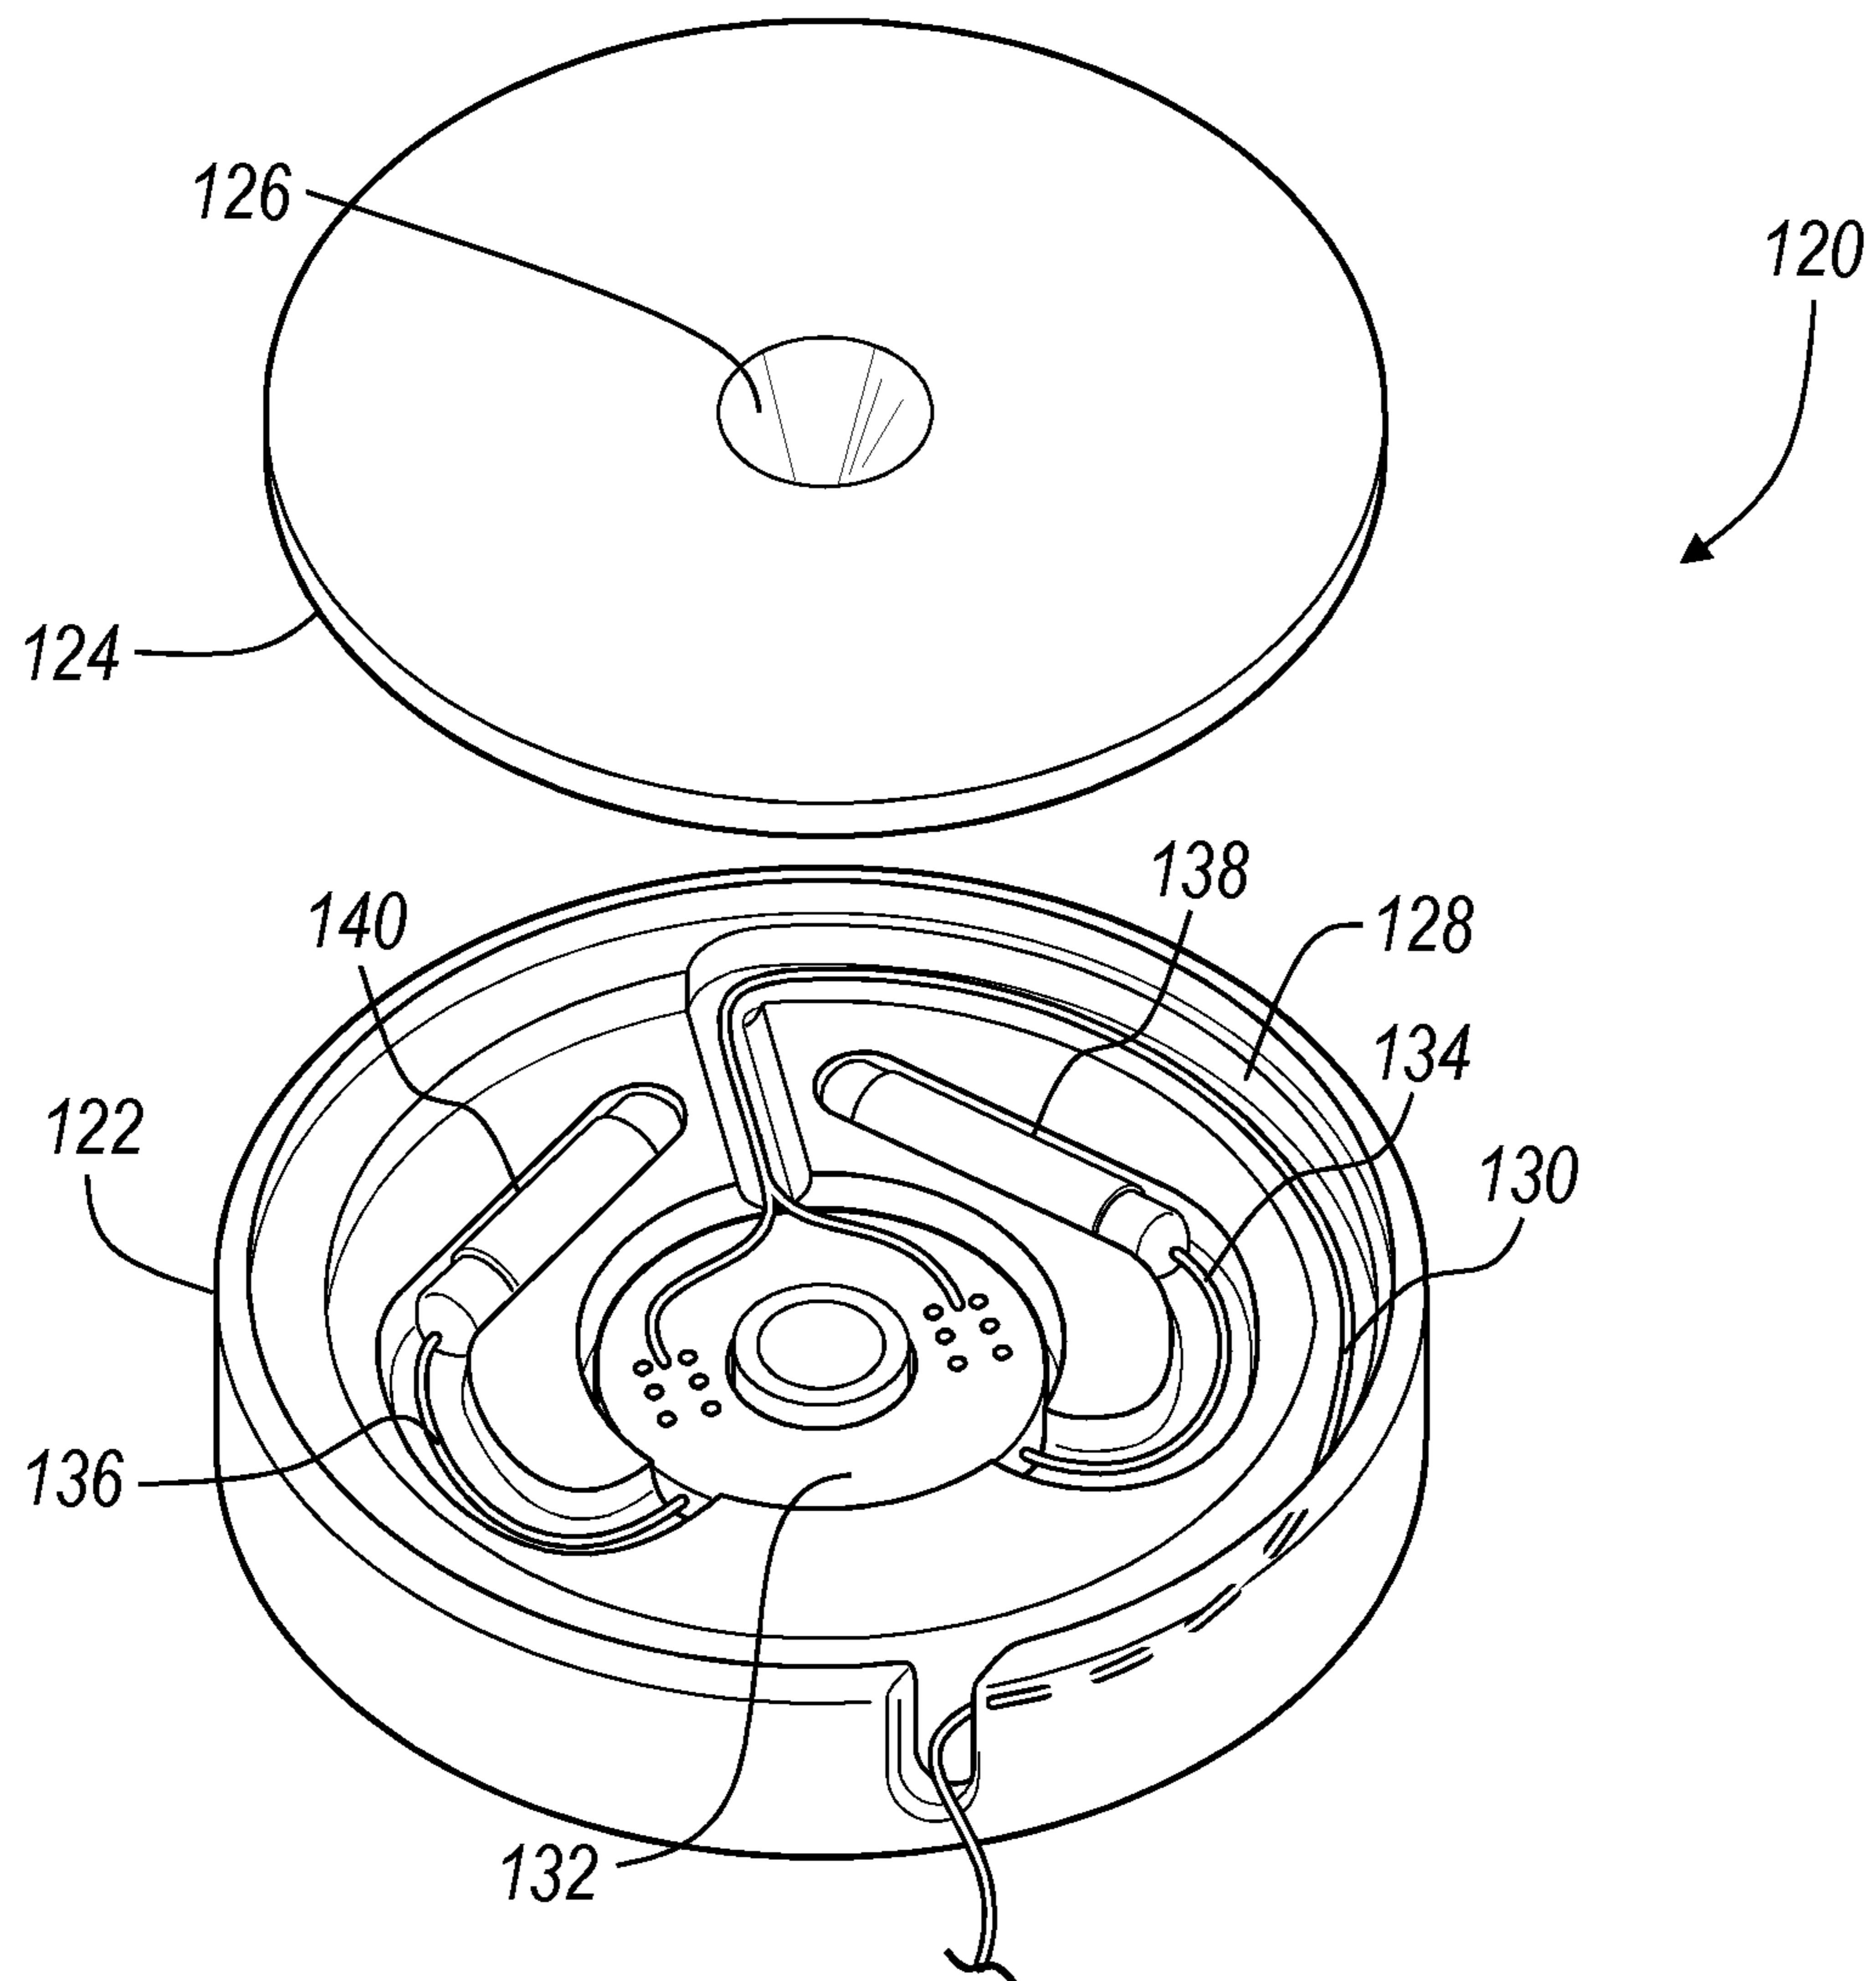
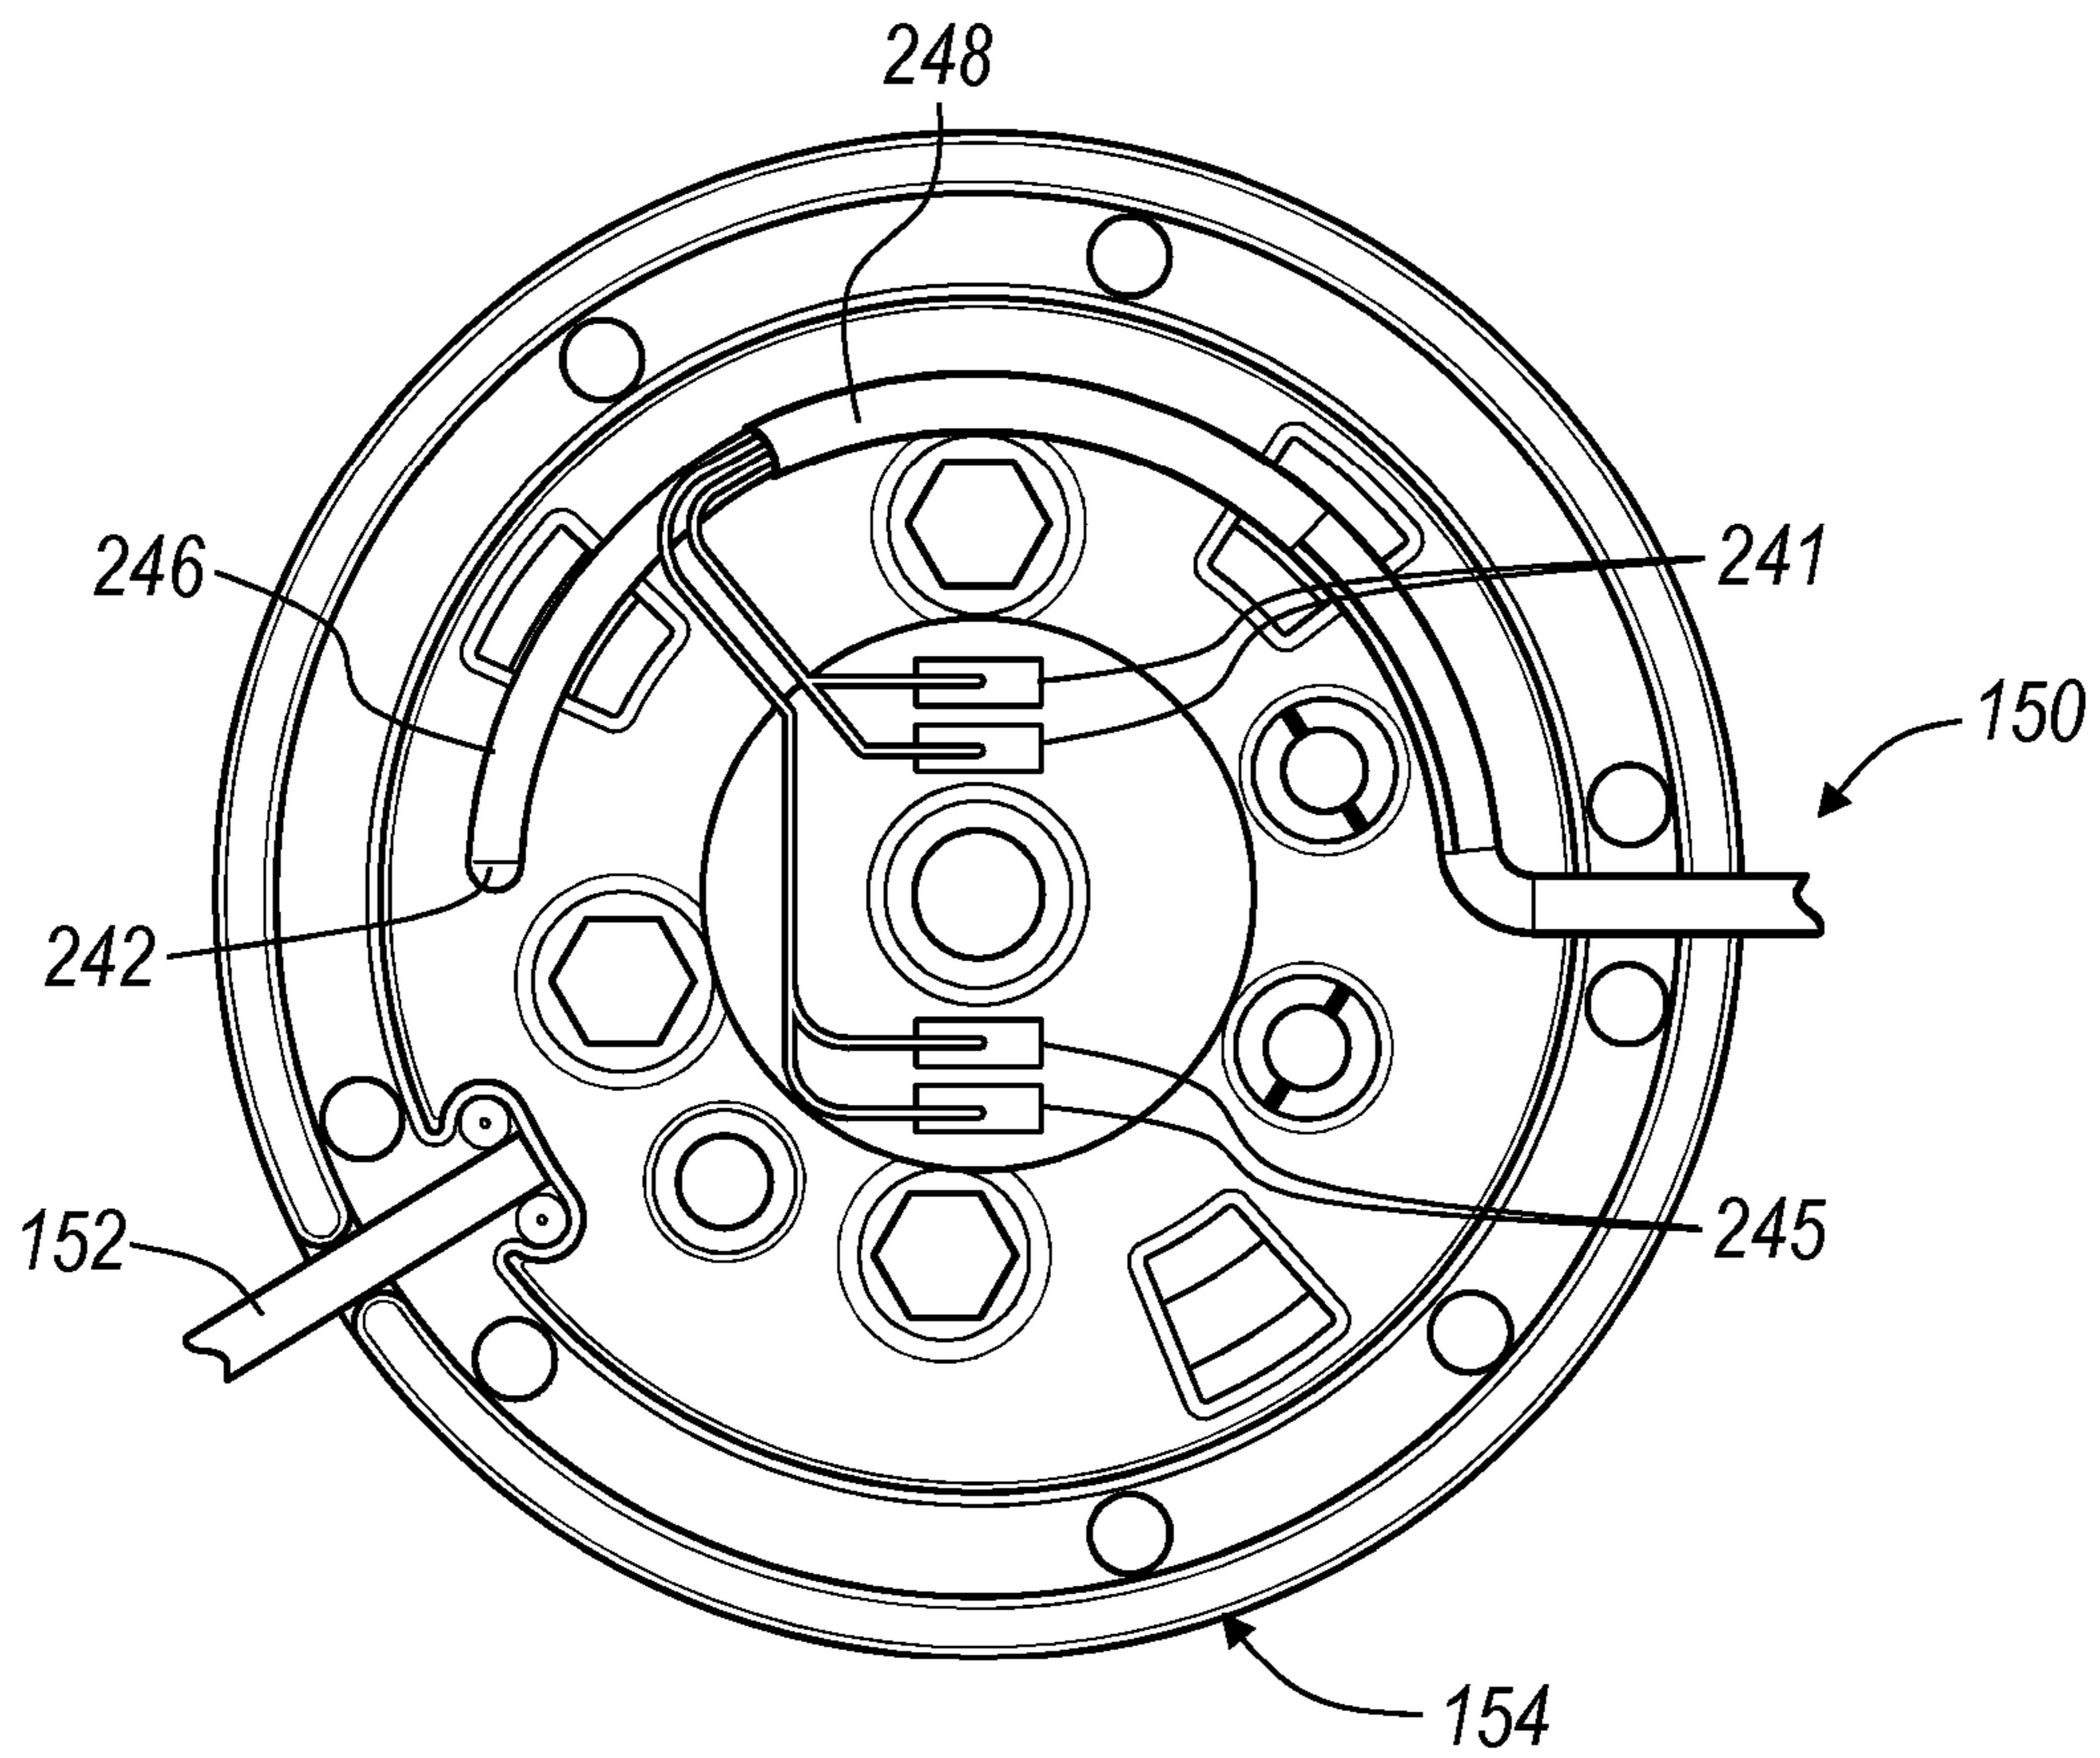
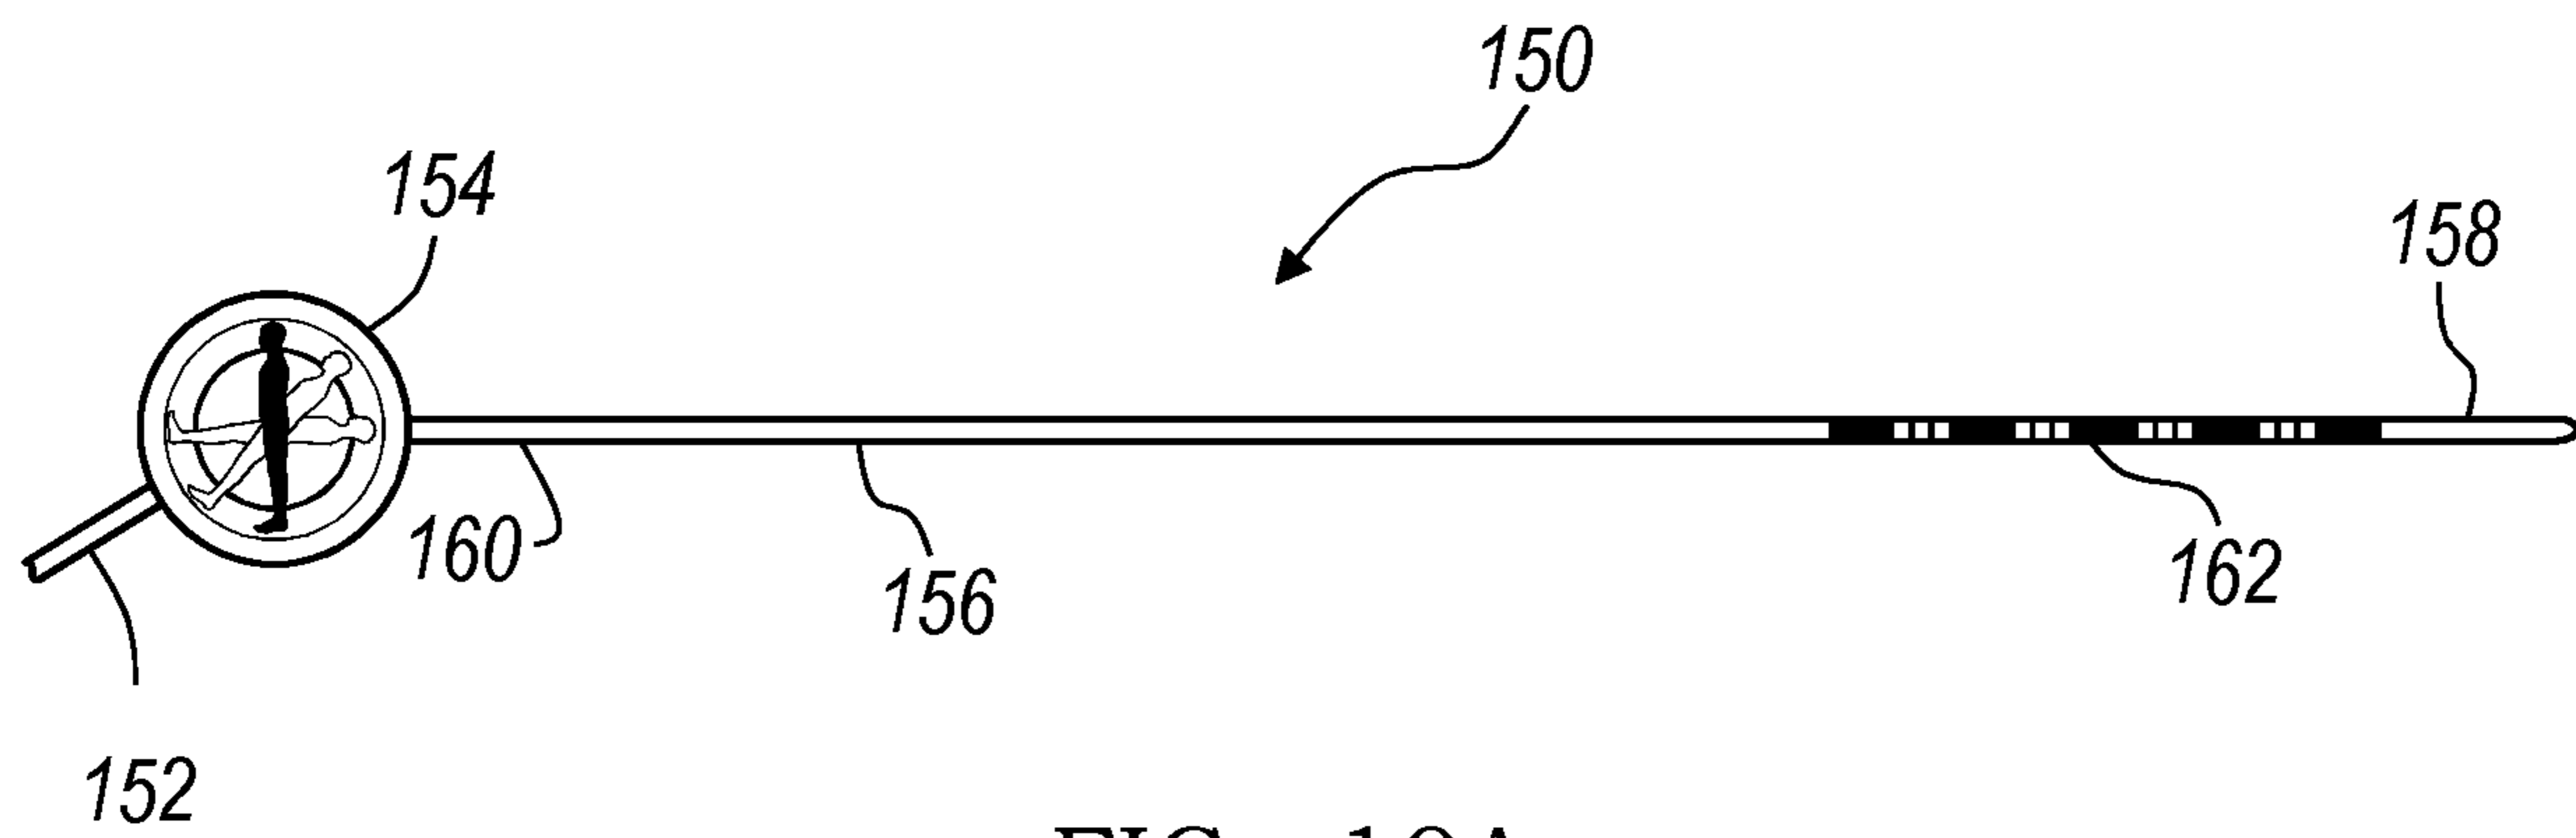
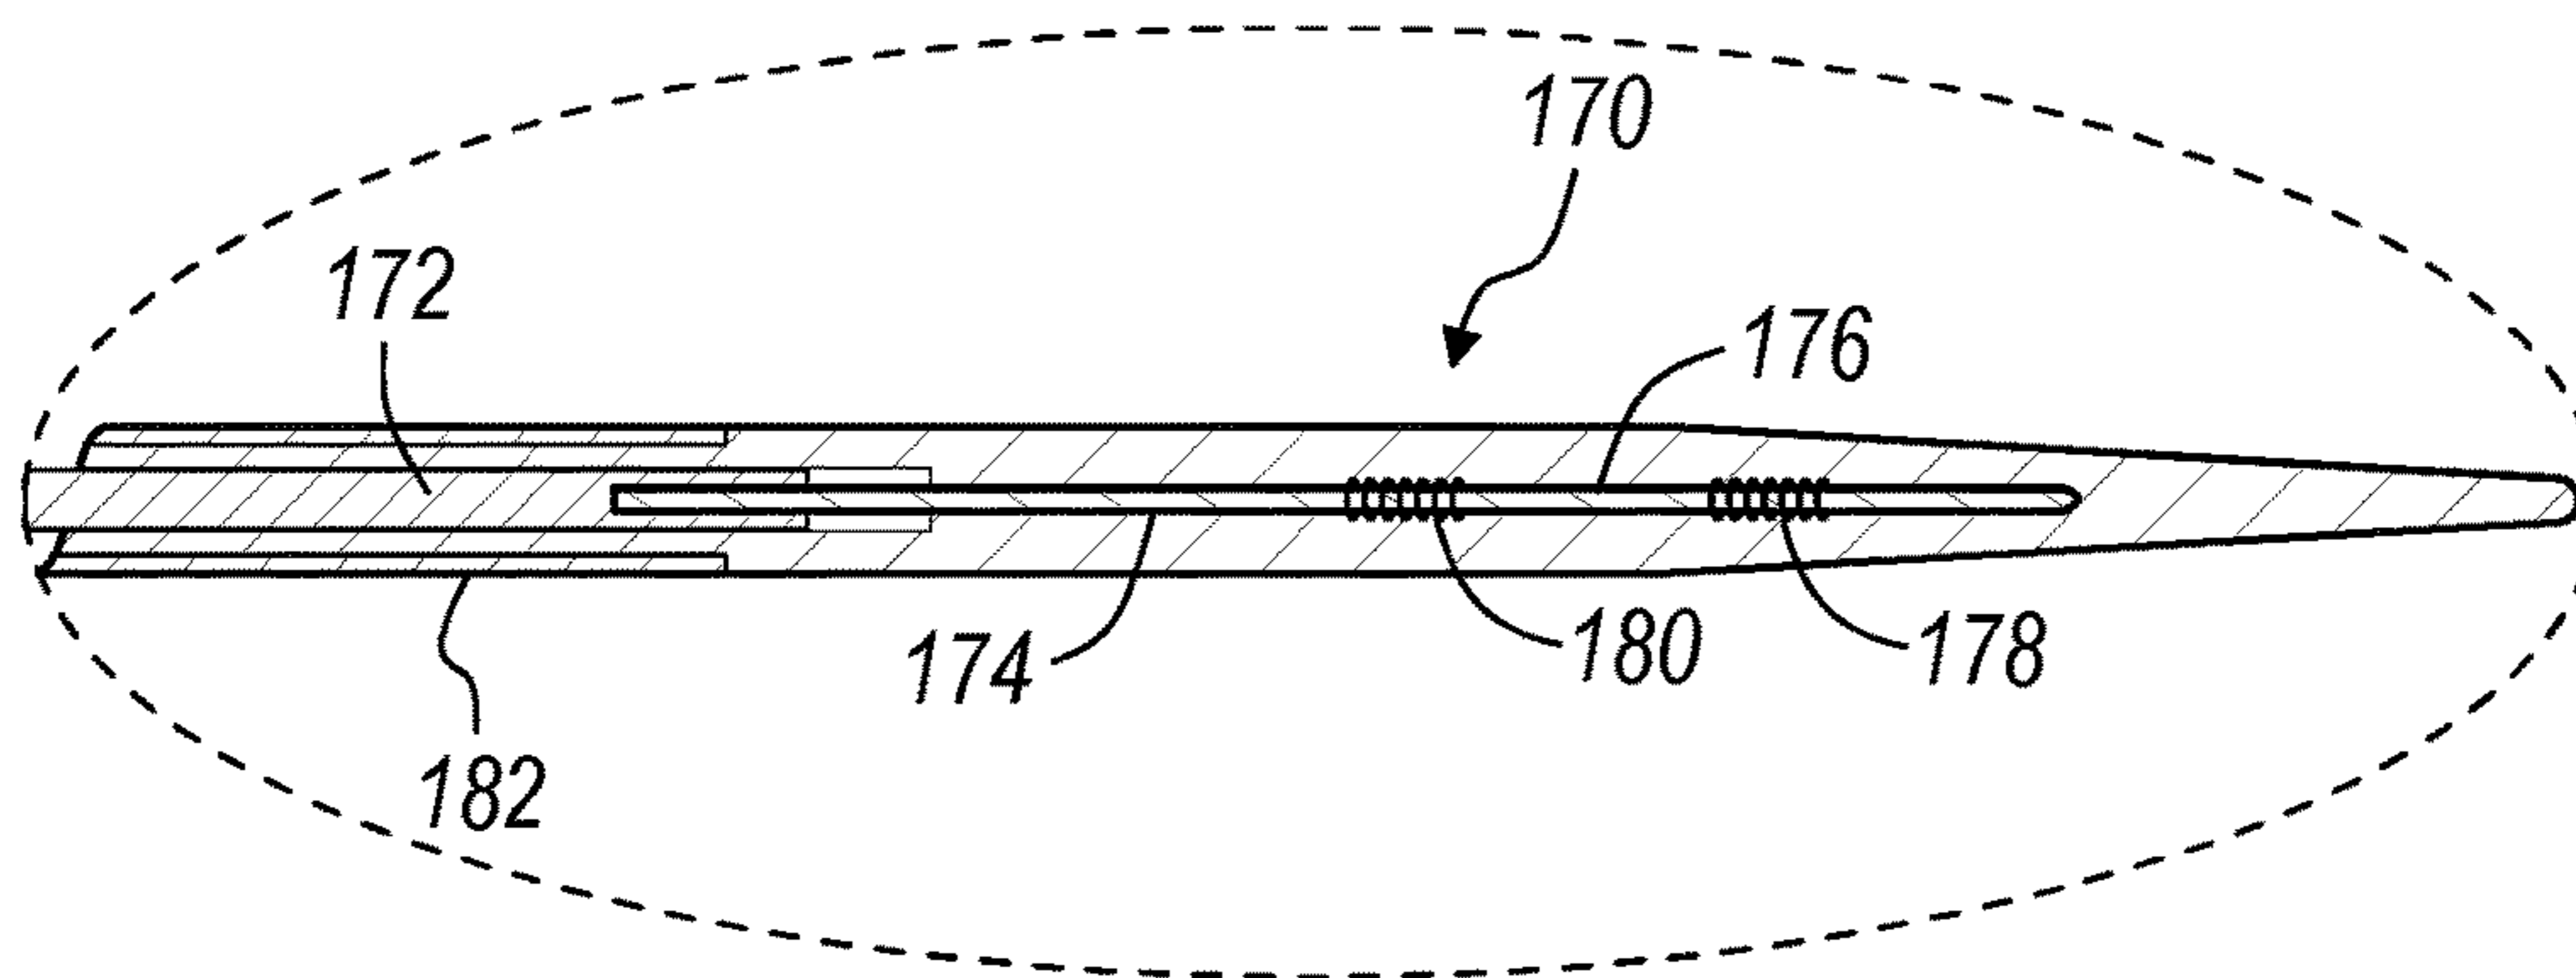
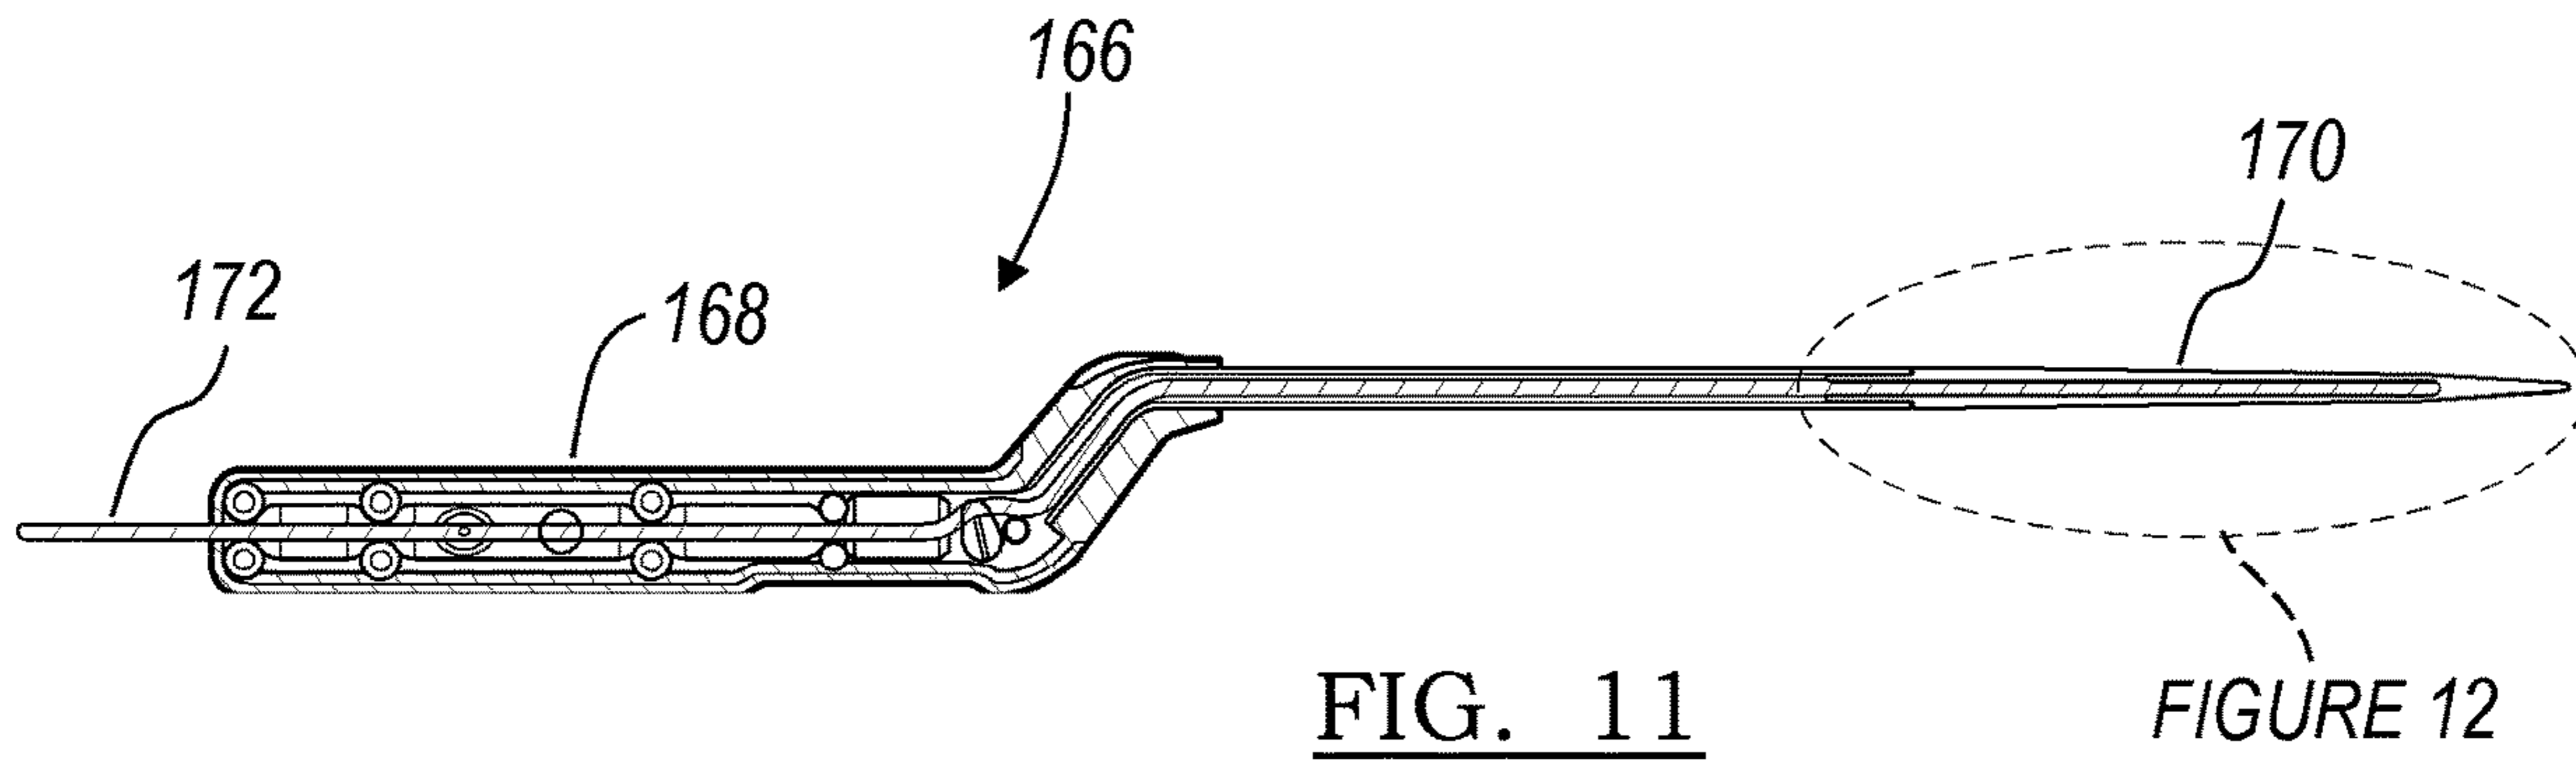


FIG. 9





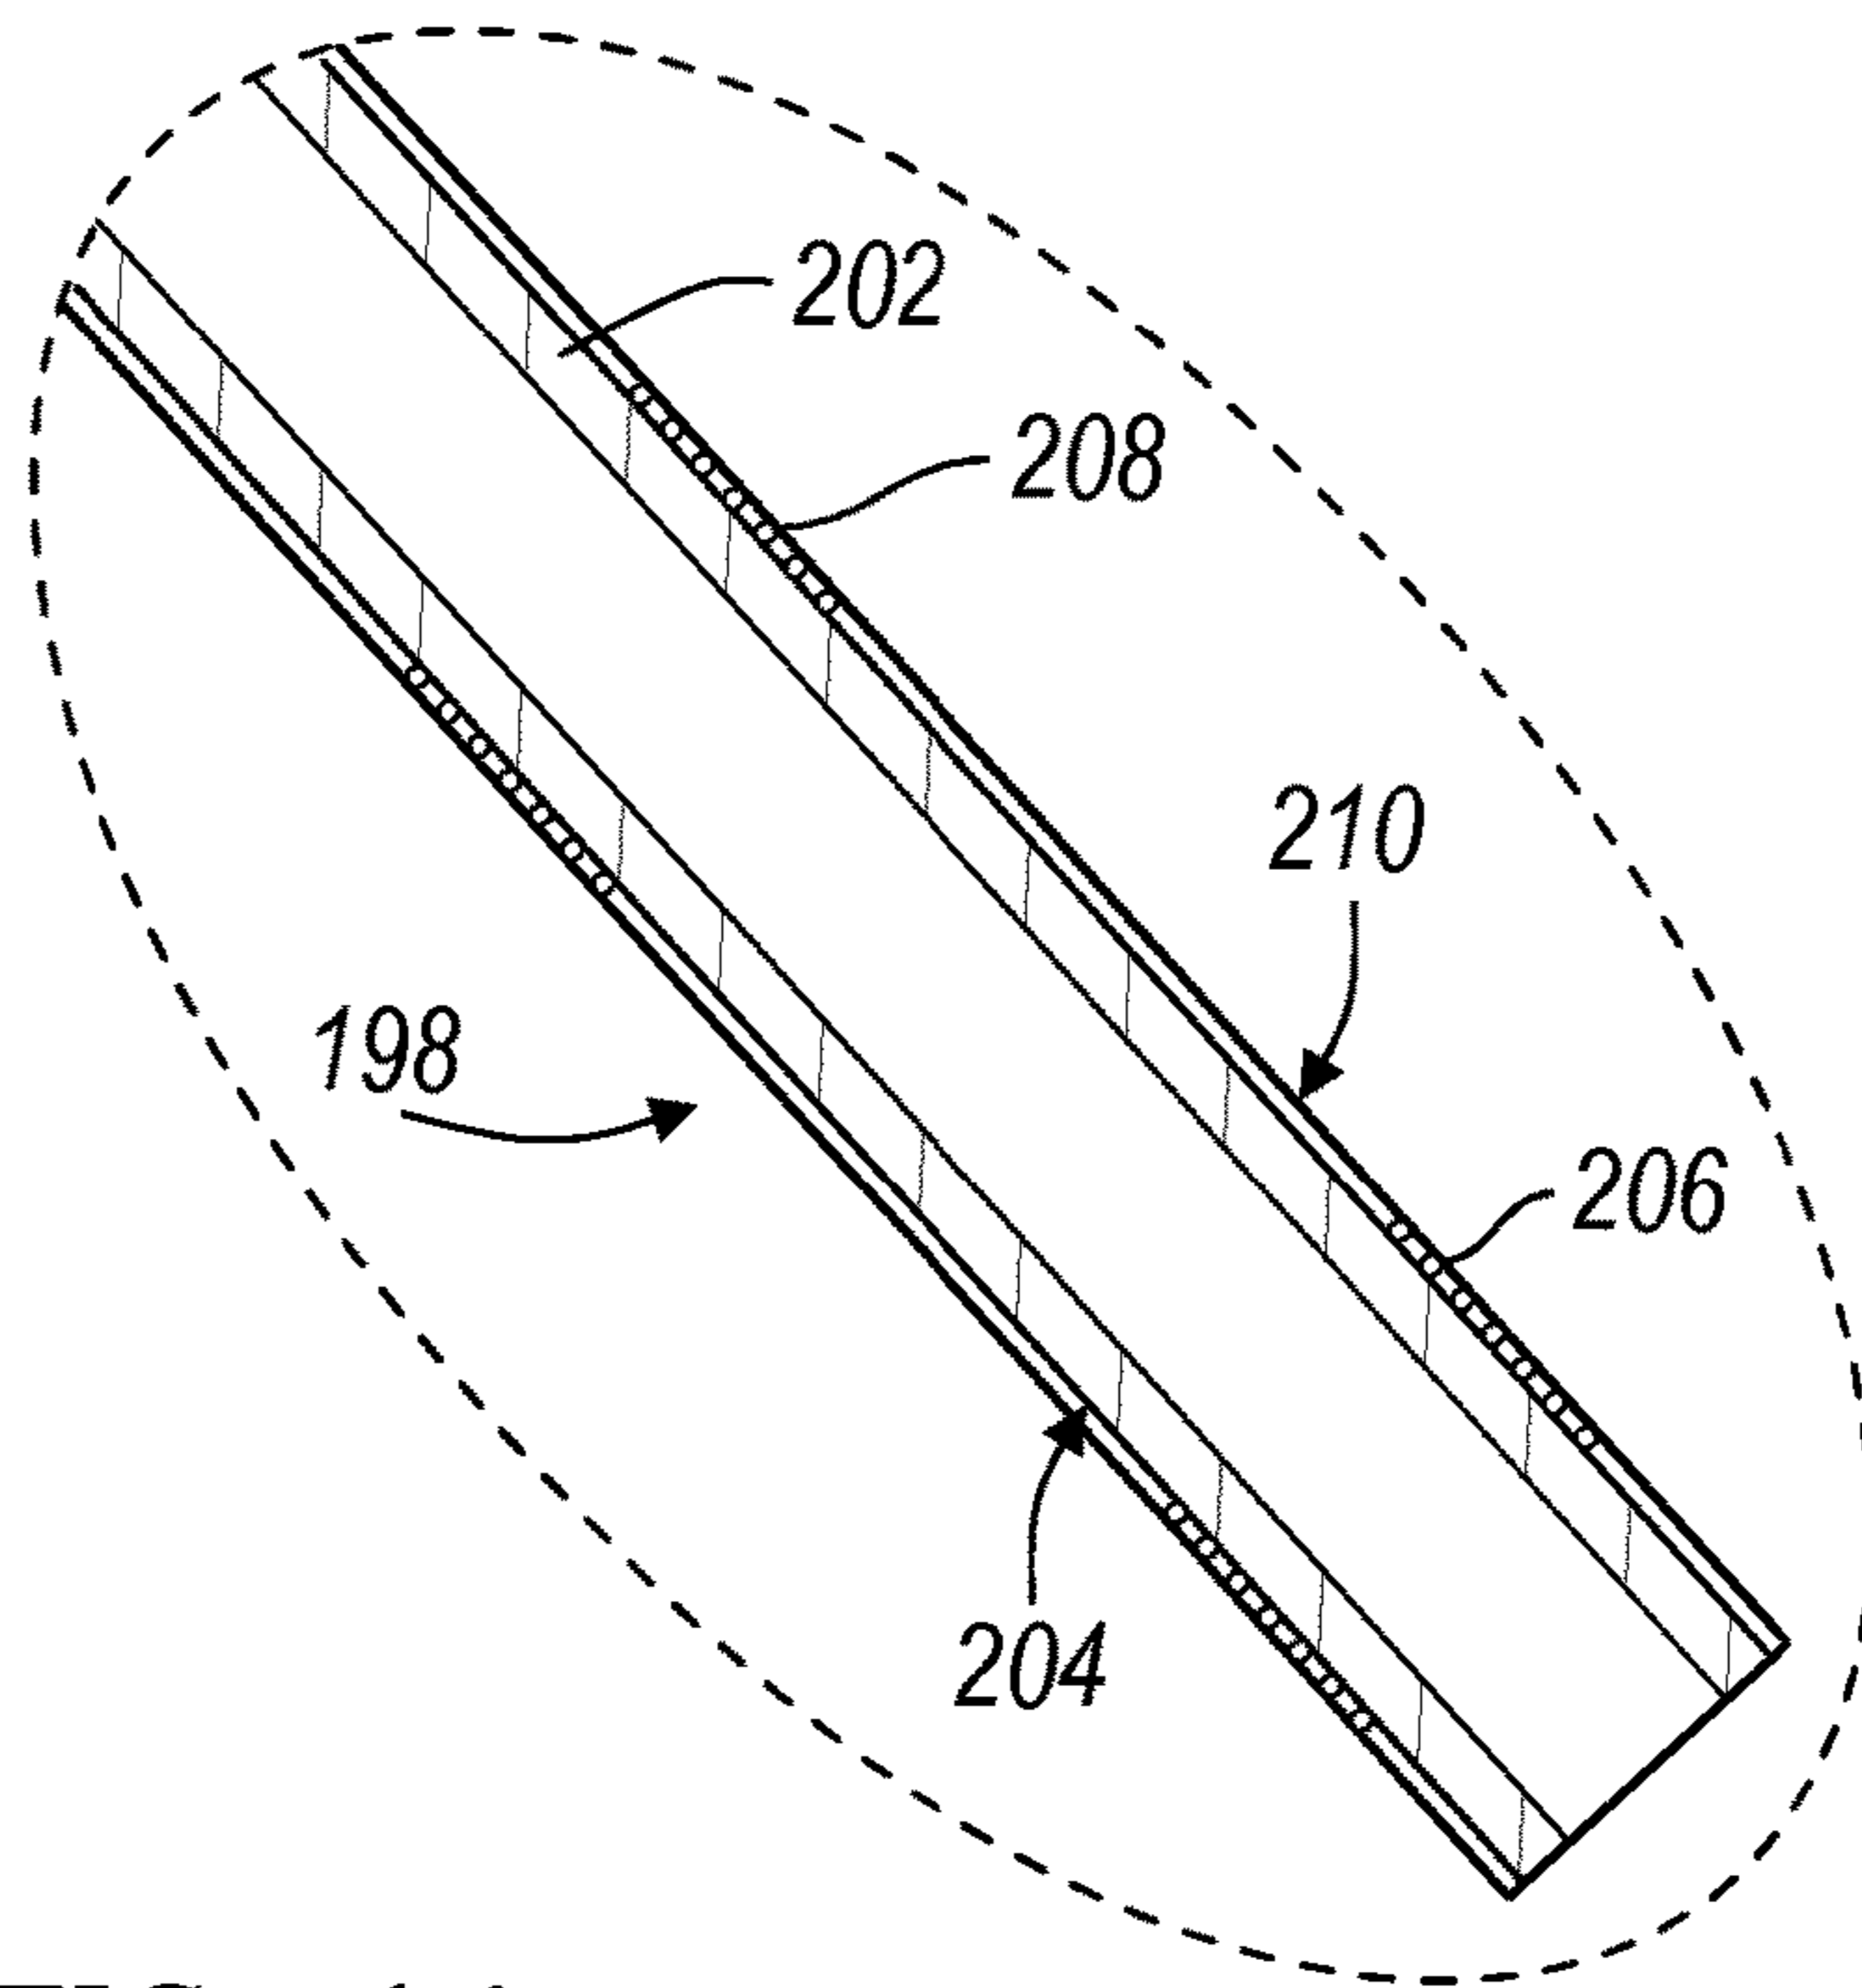
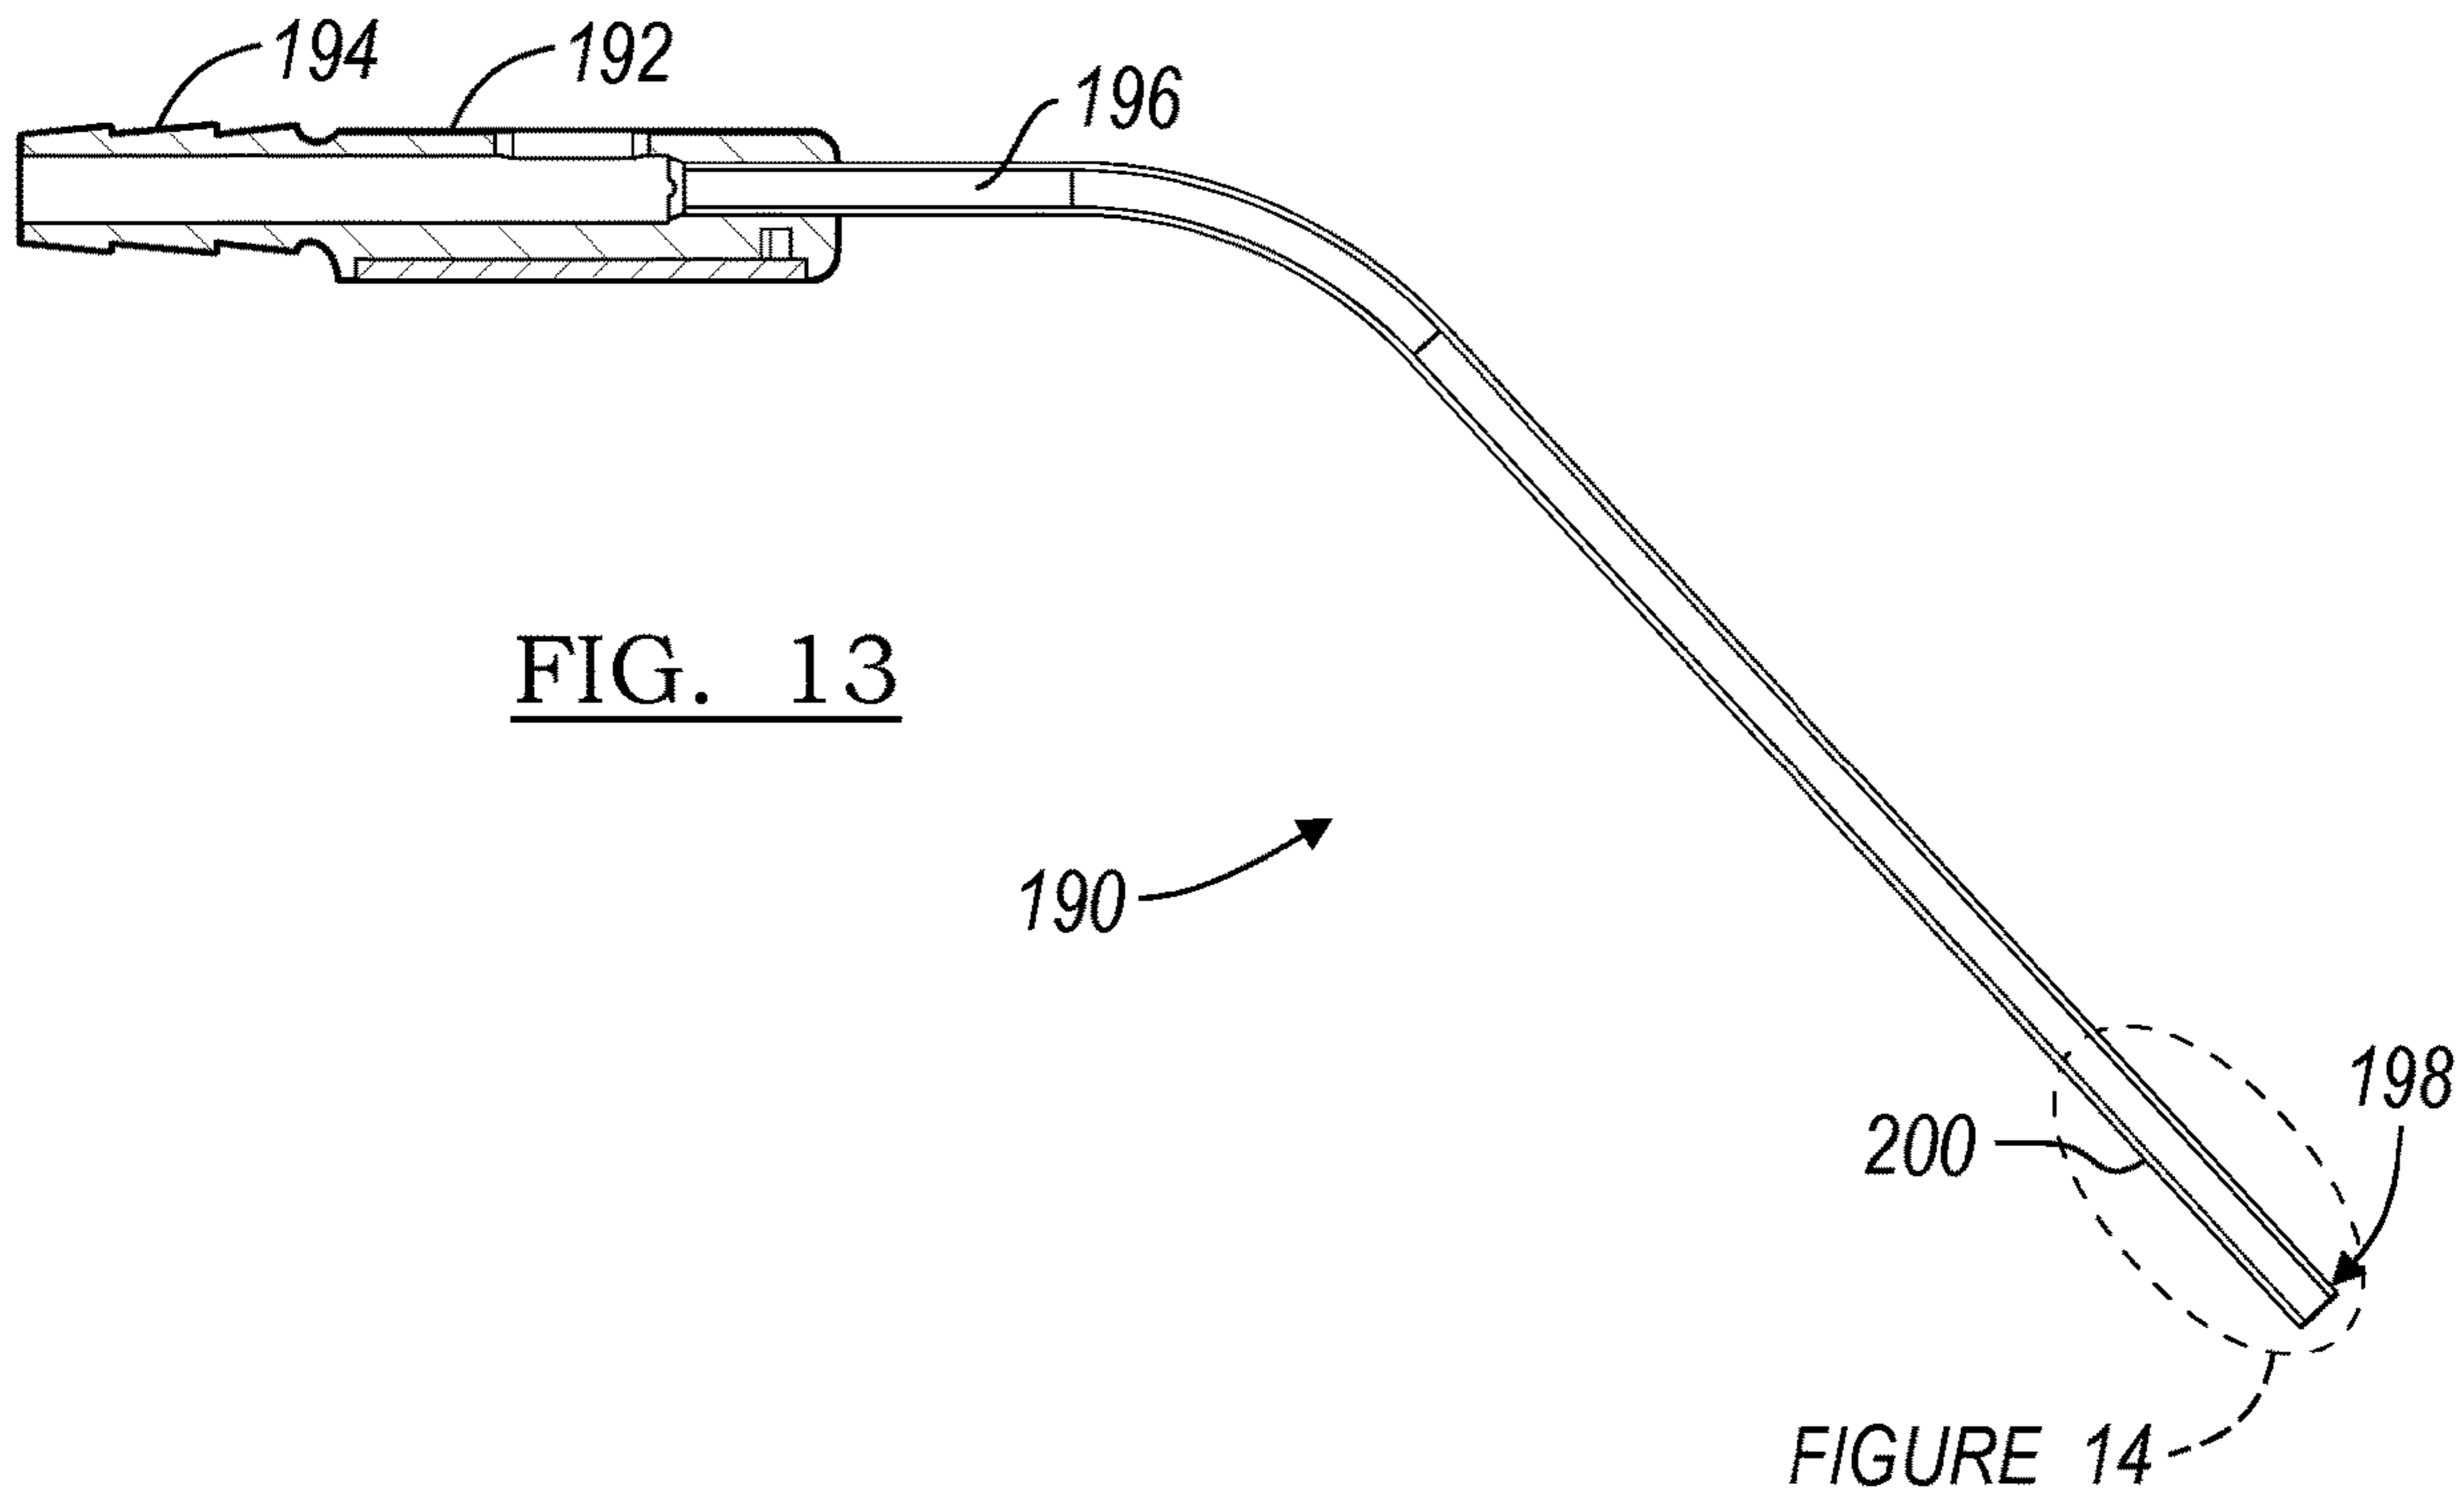


FIG. 14

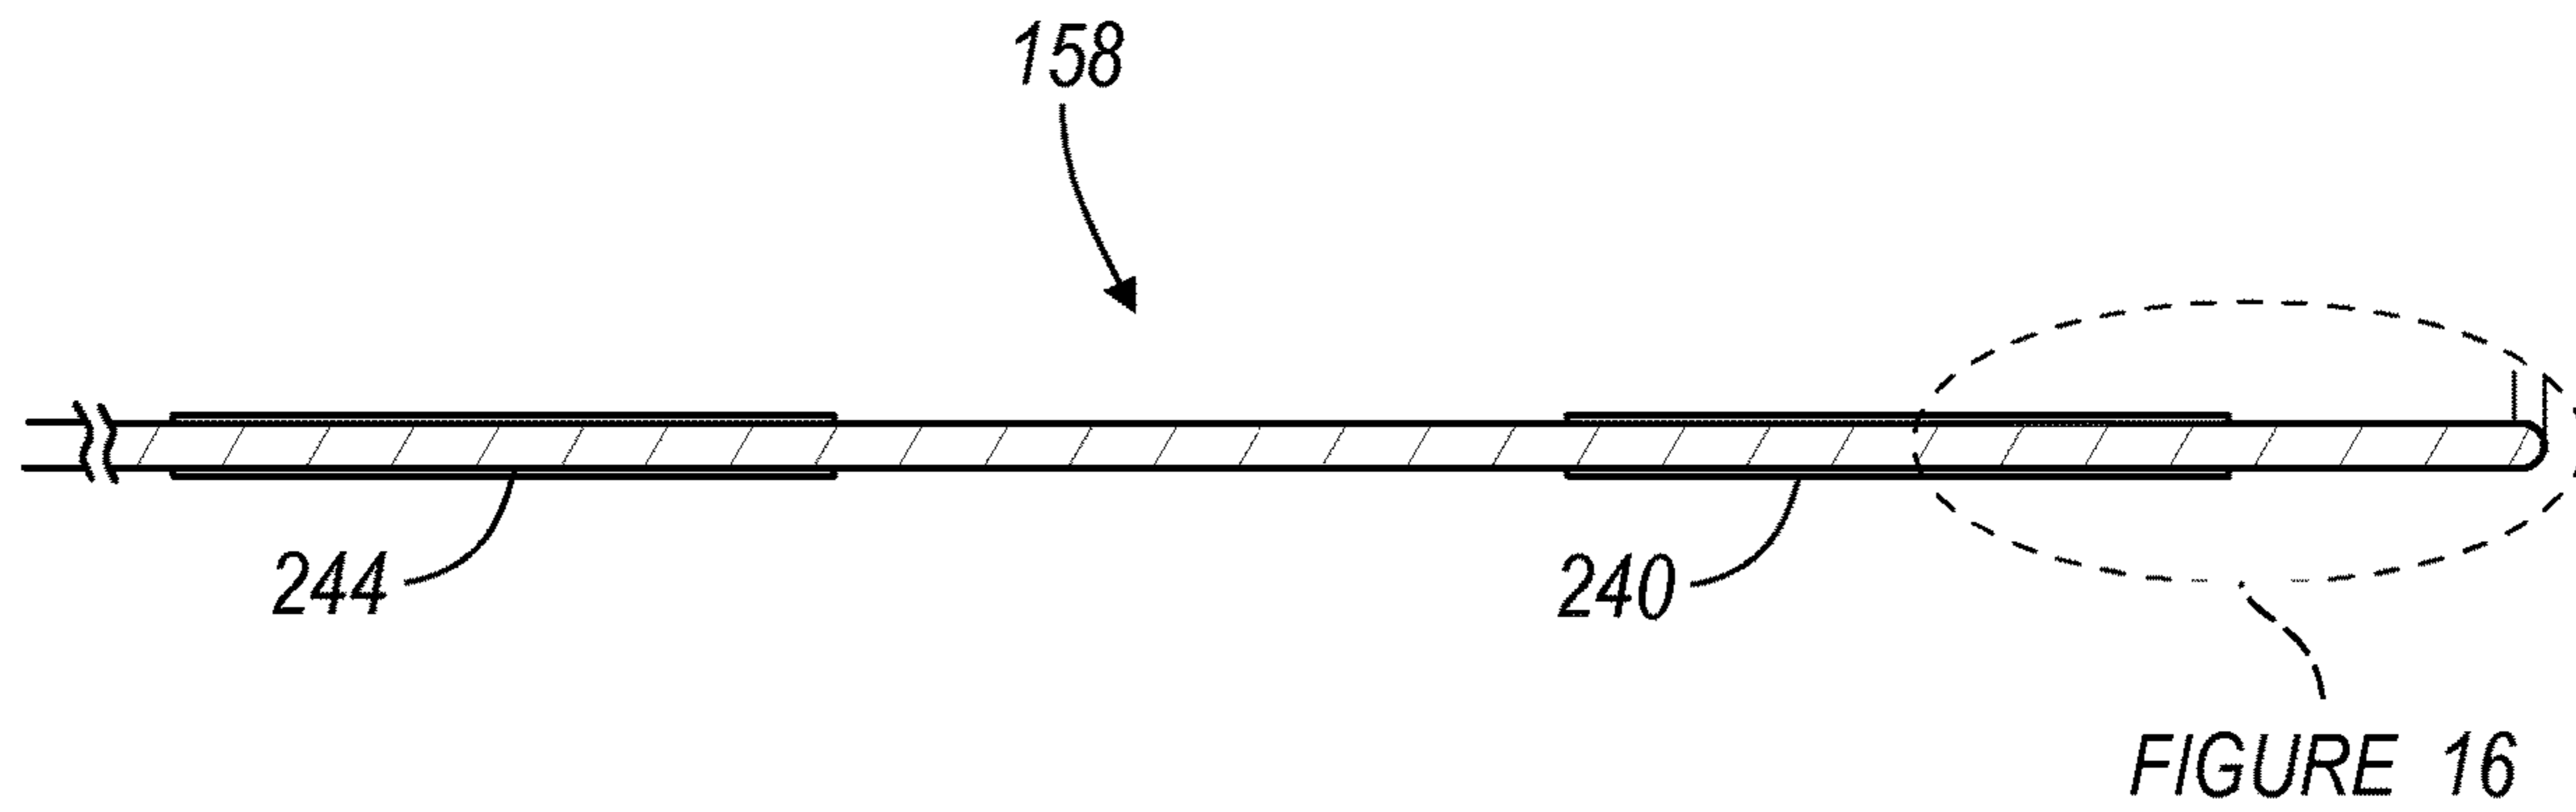


FIG. 15

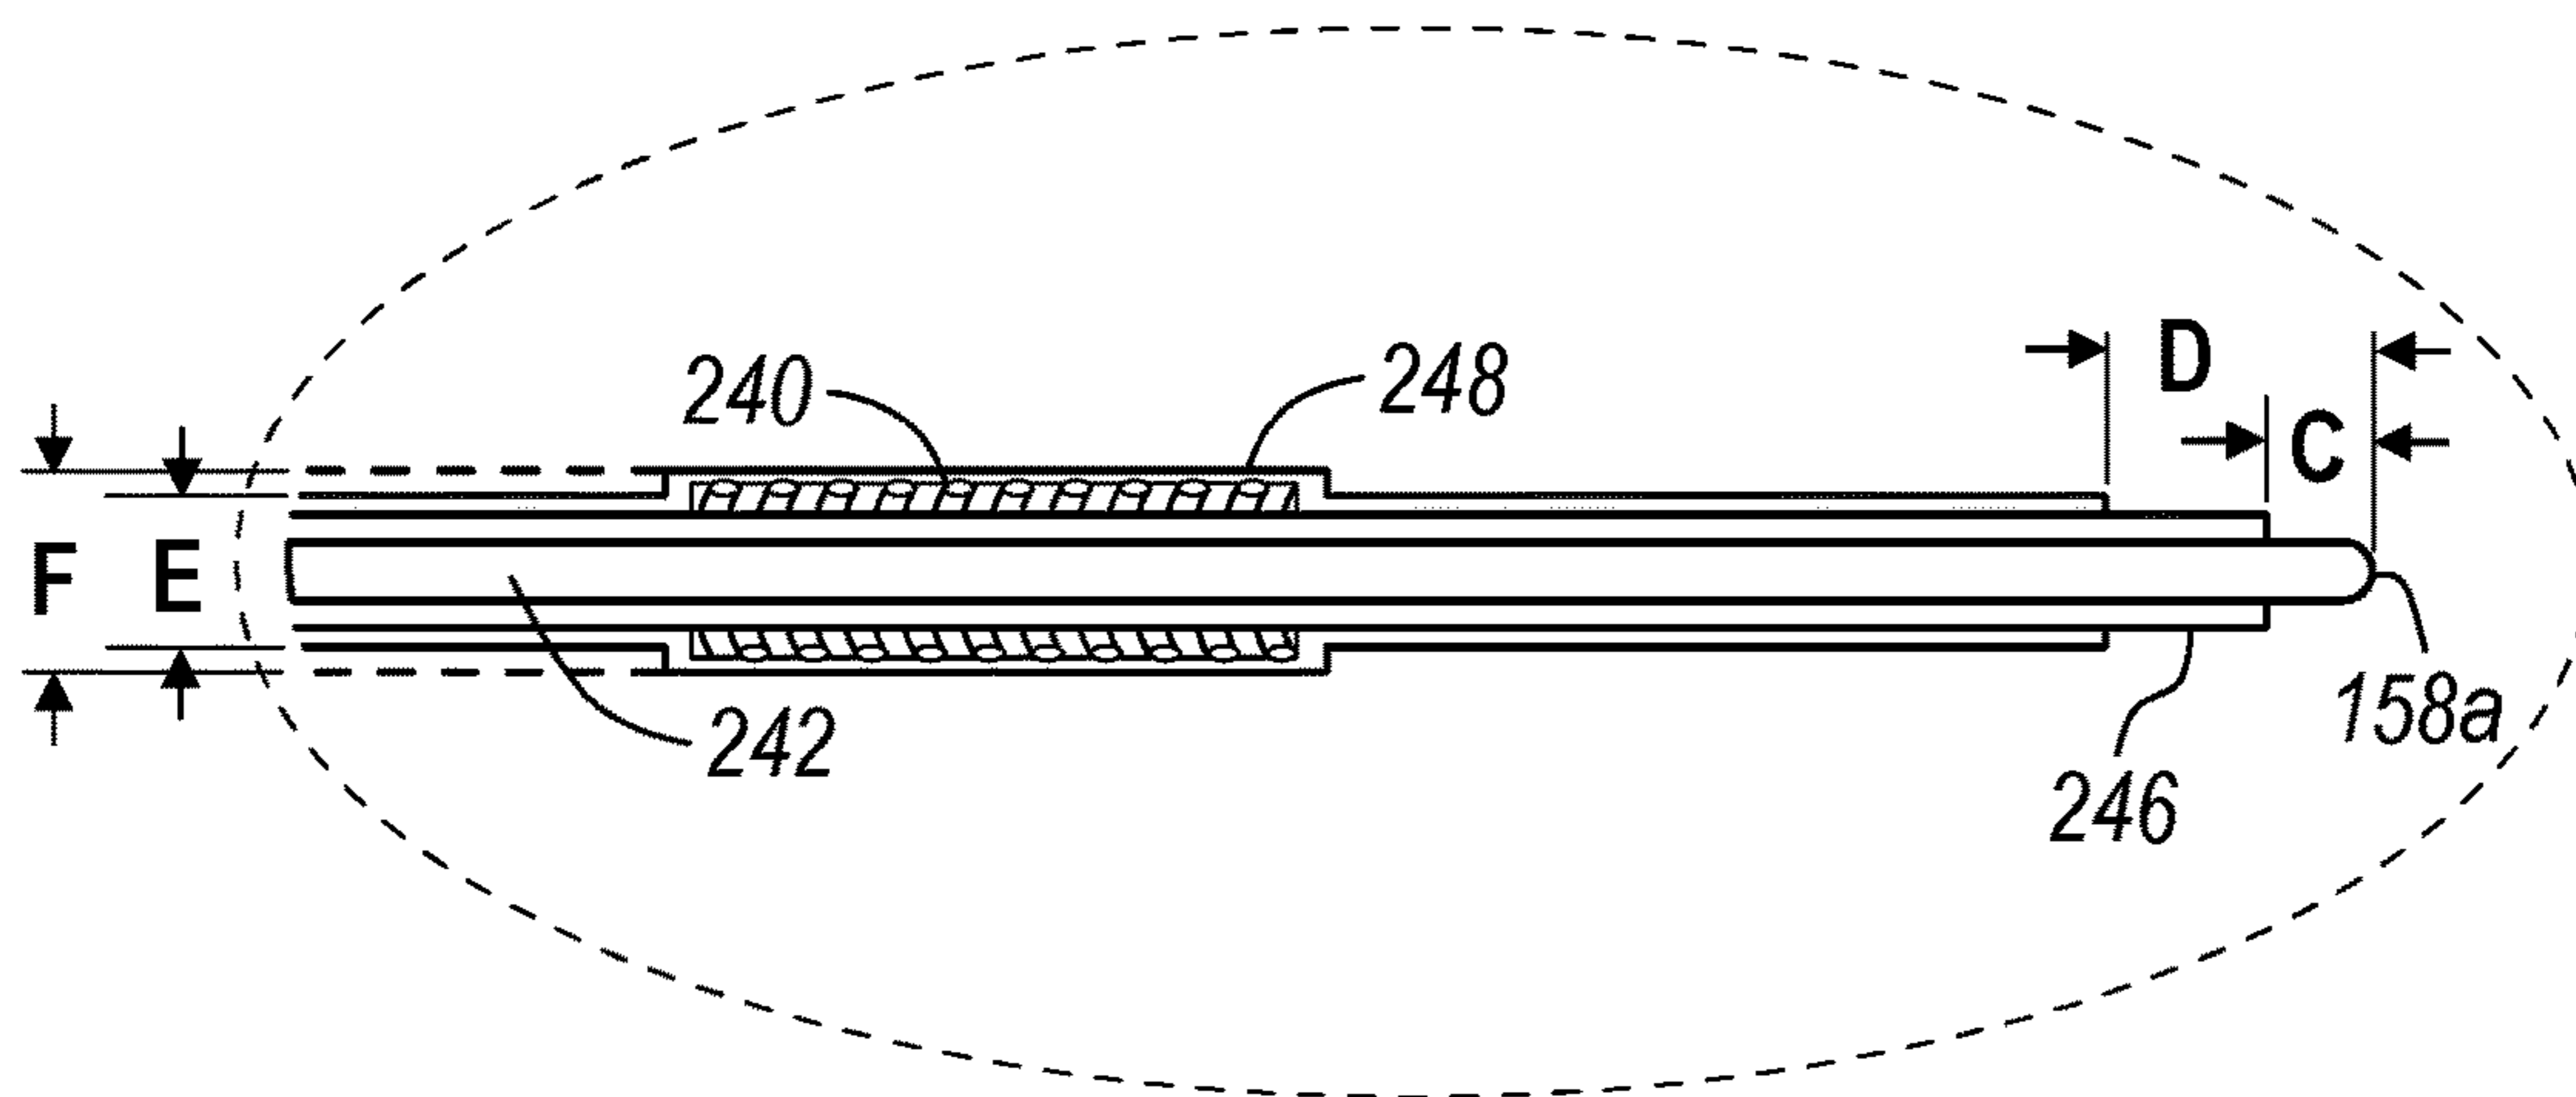


FIG. 16

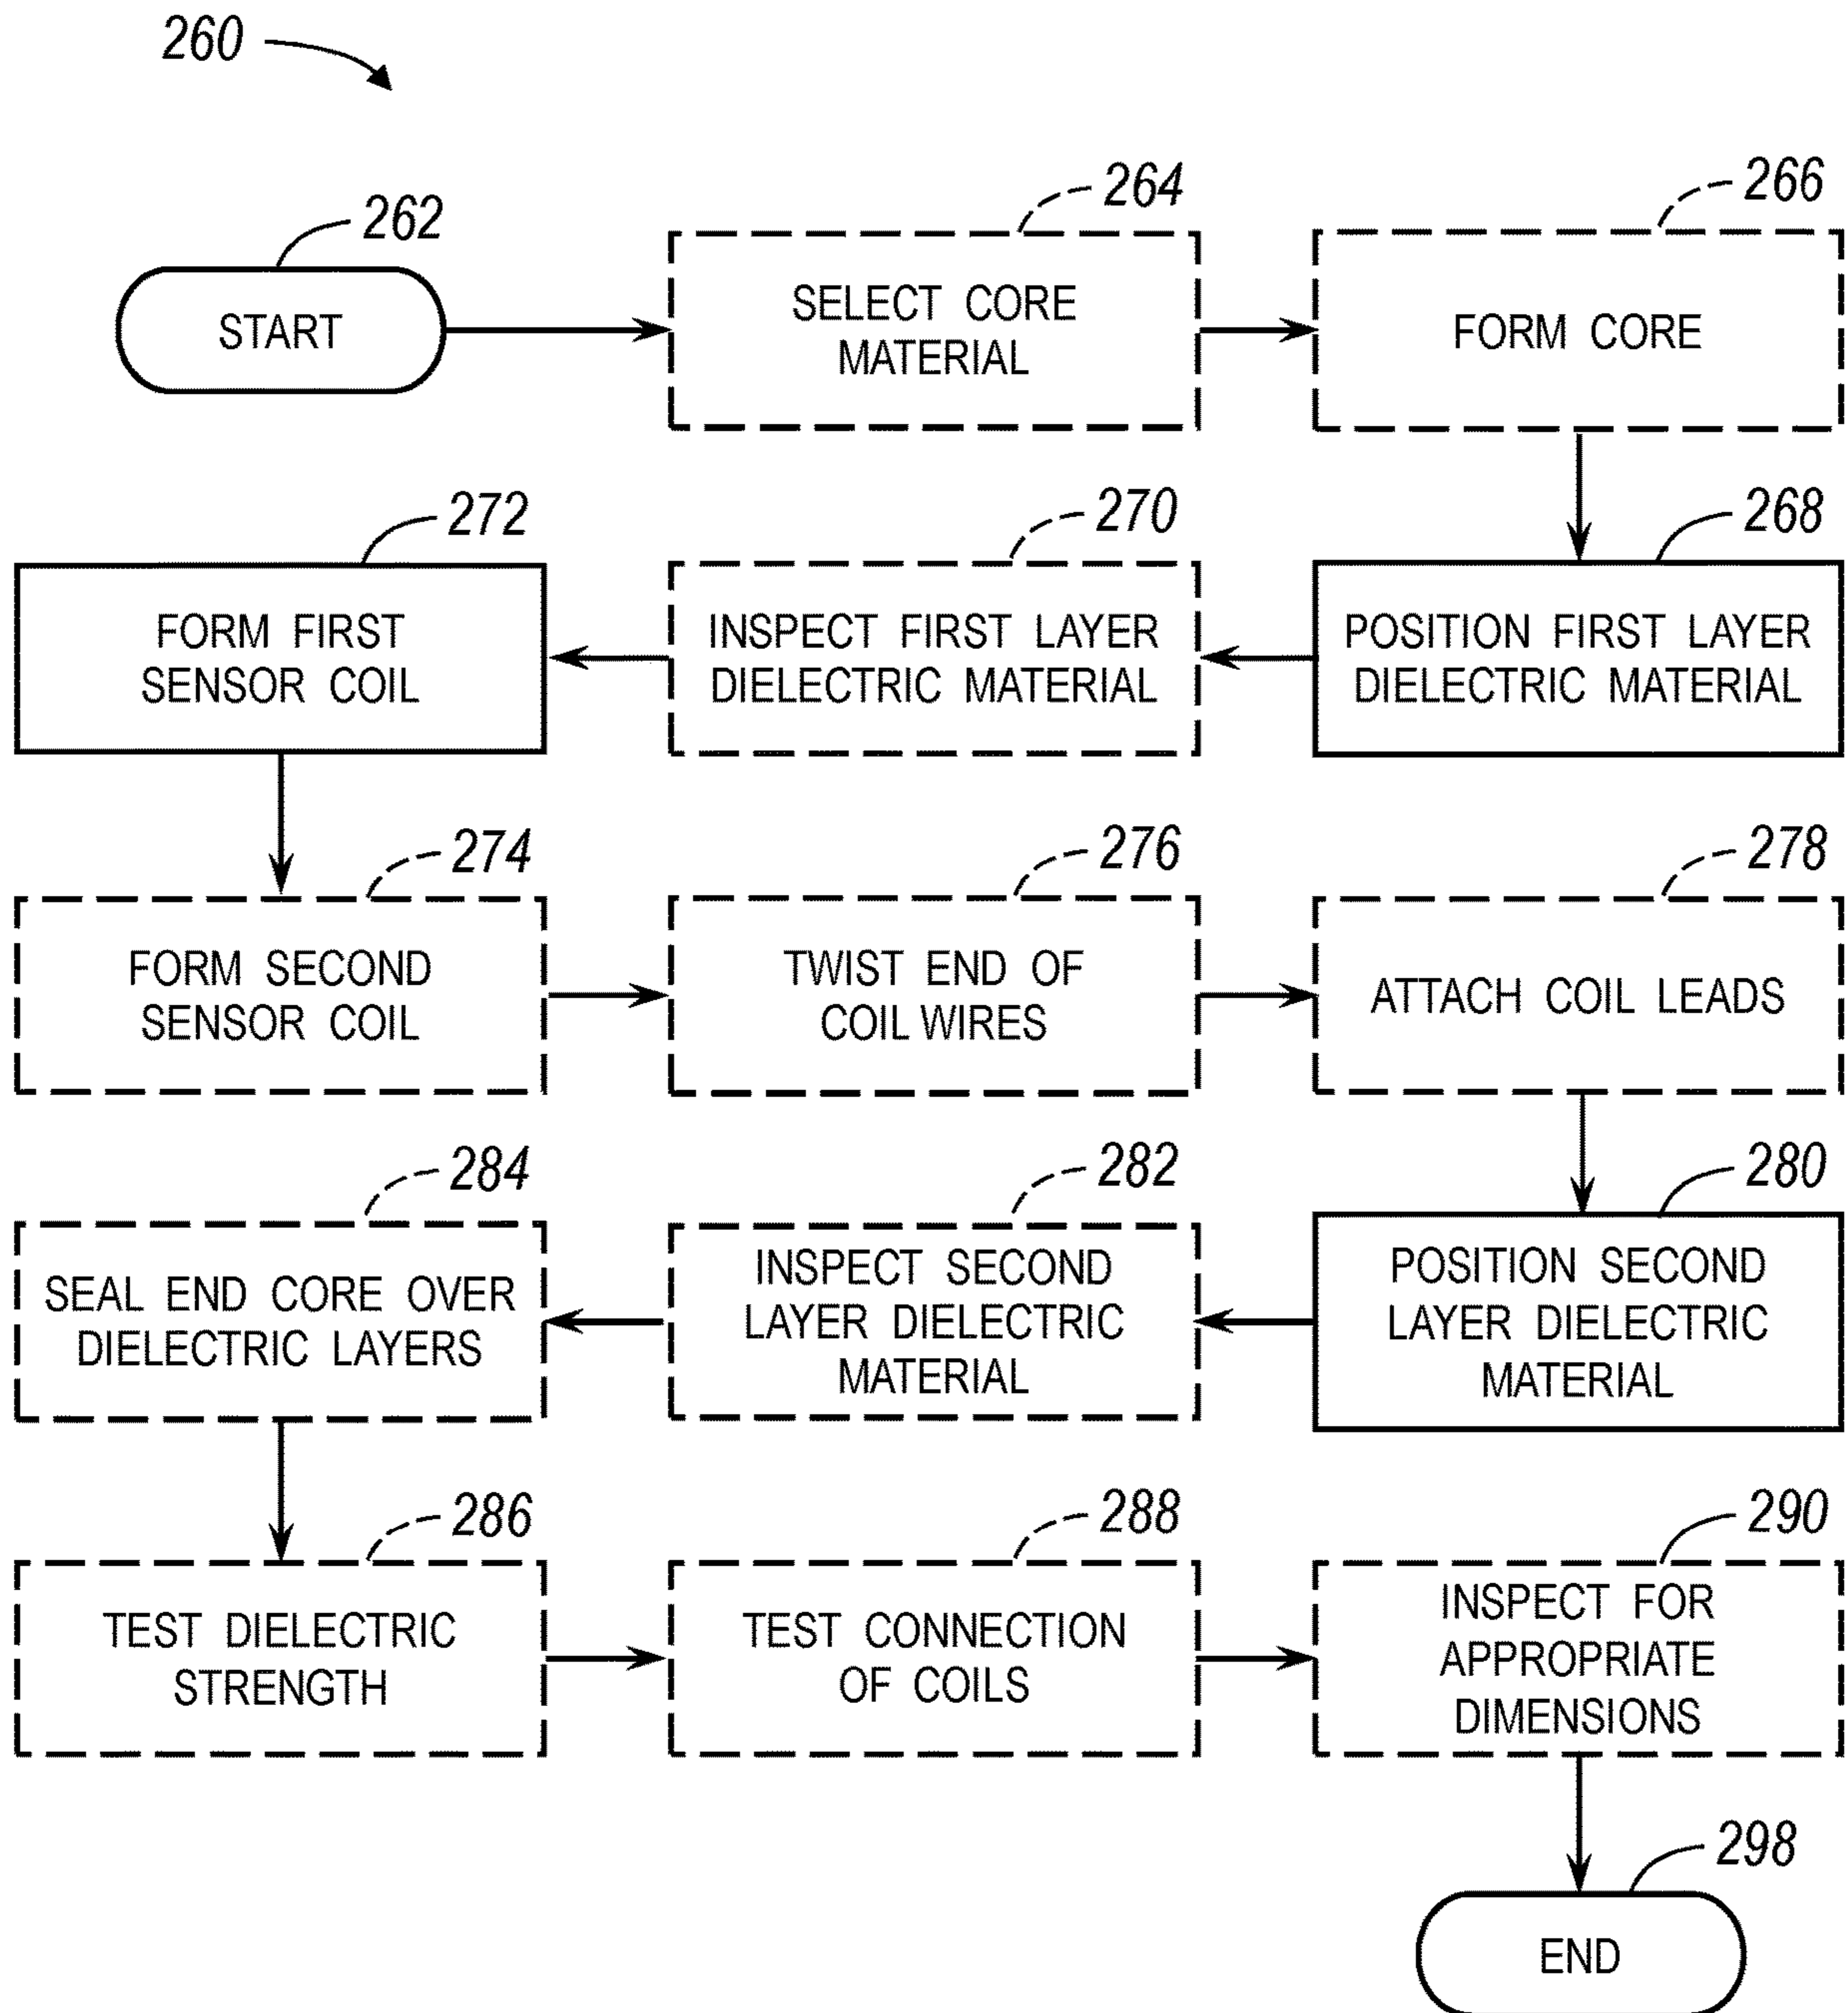


FIG. 17

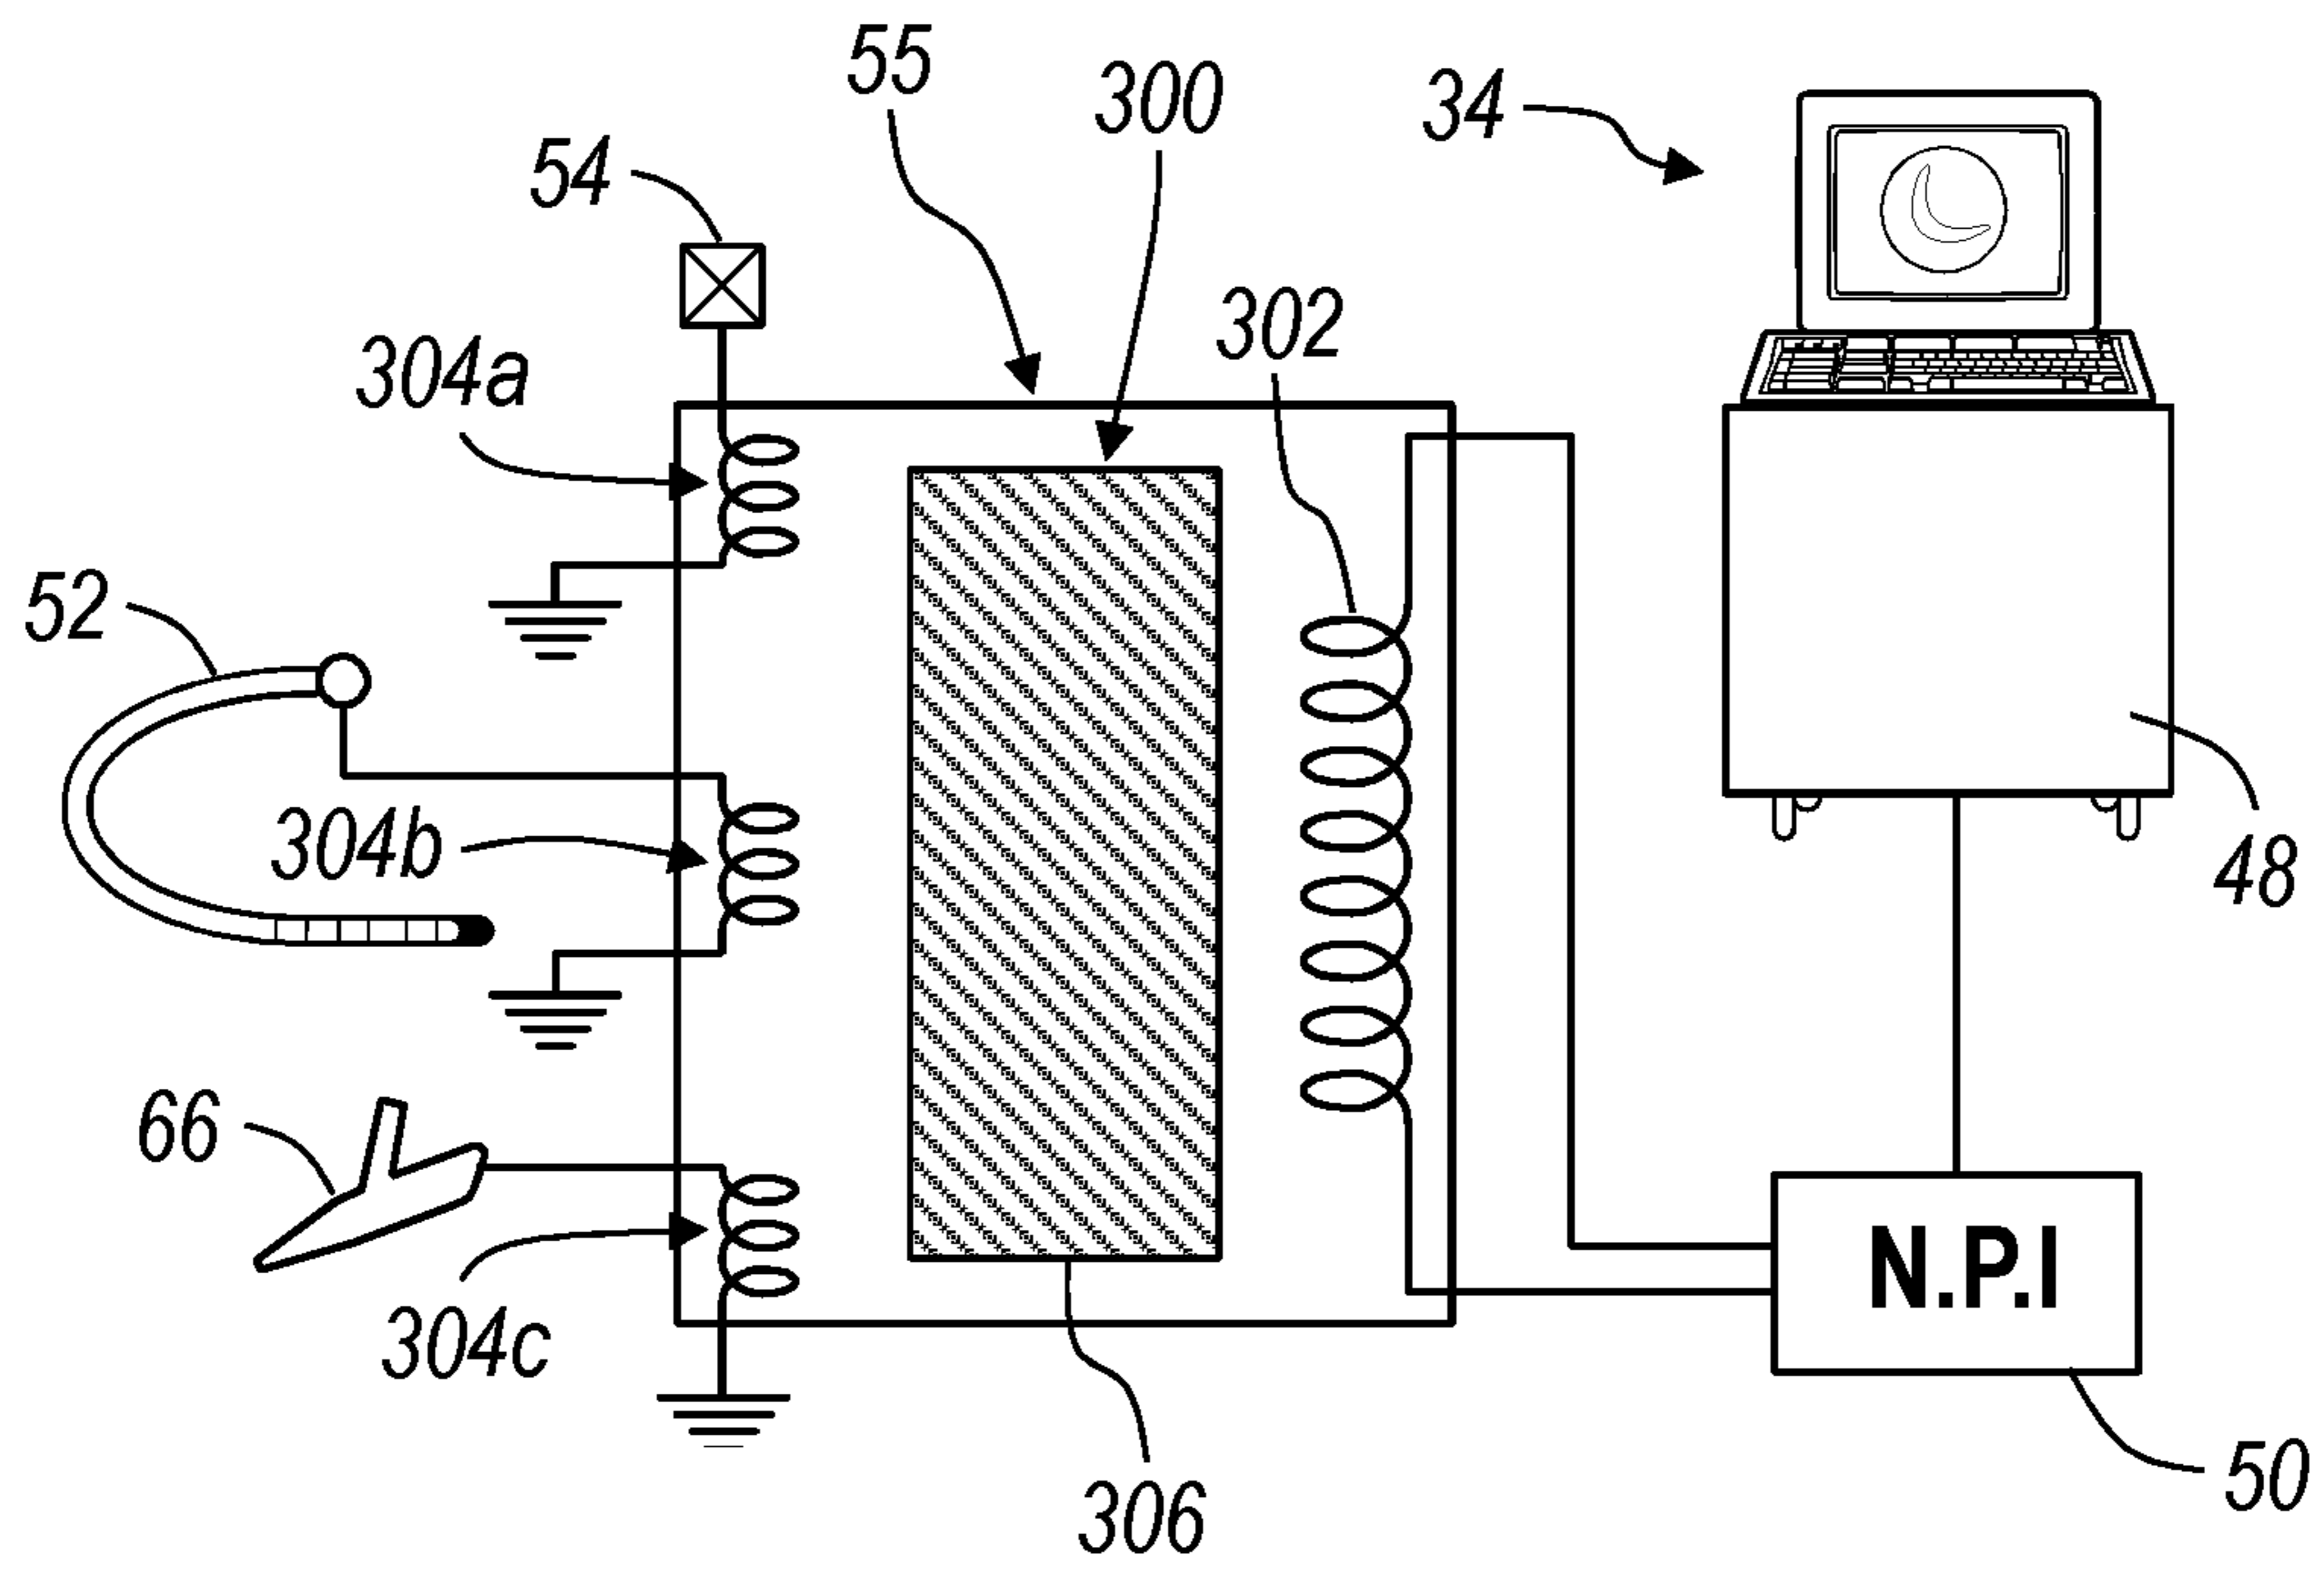


FIG. 18

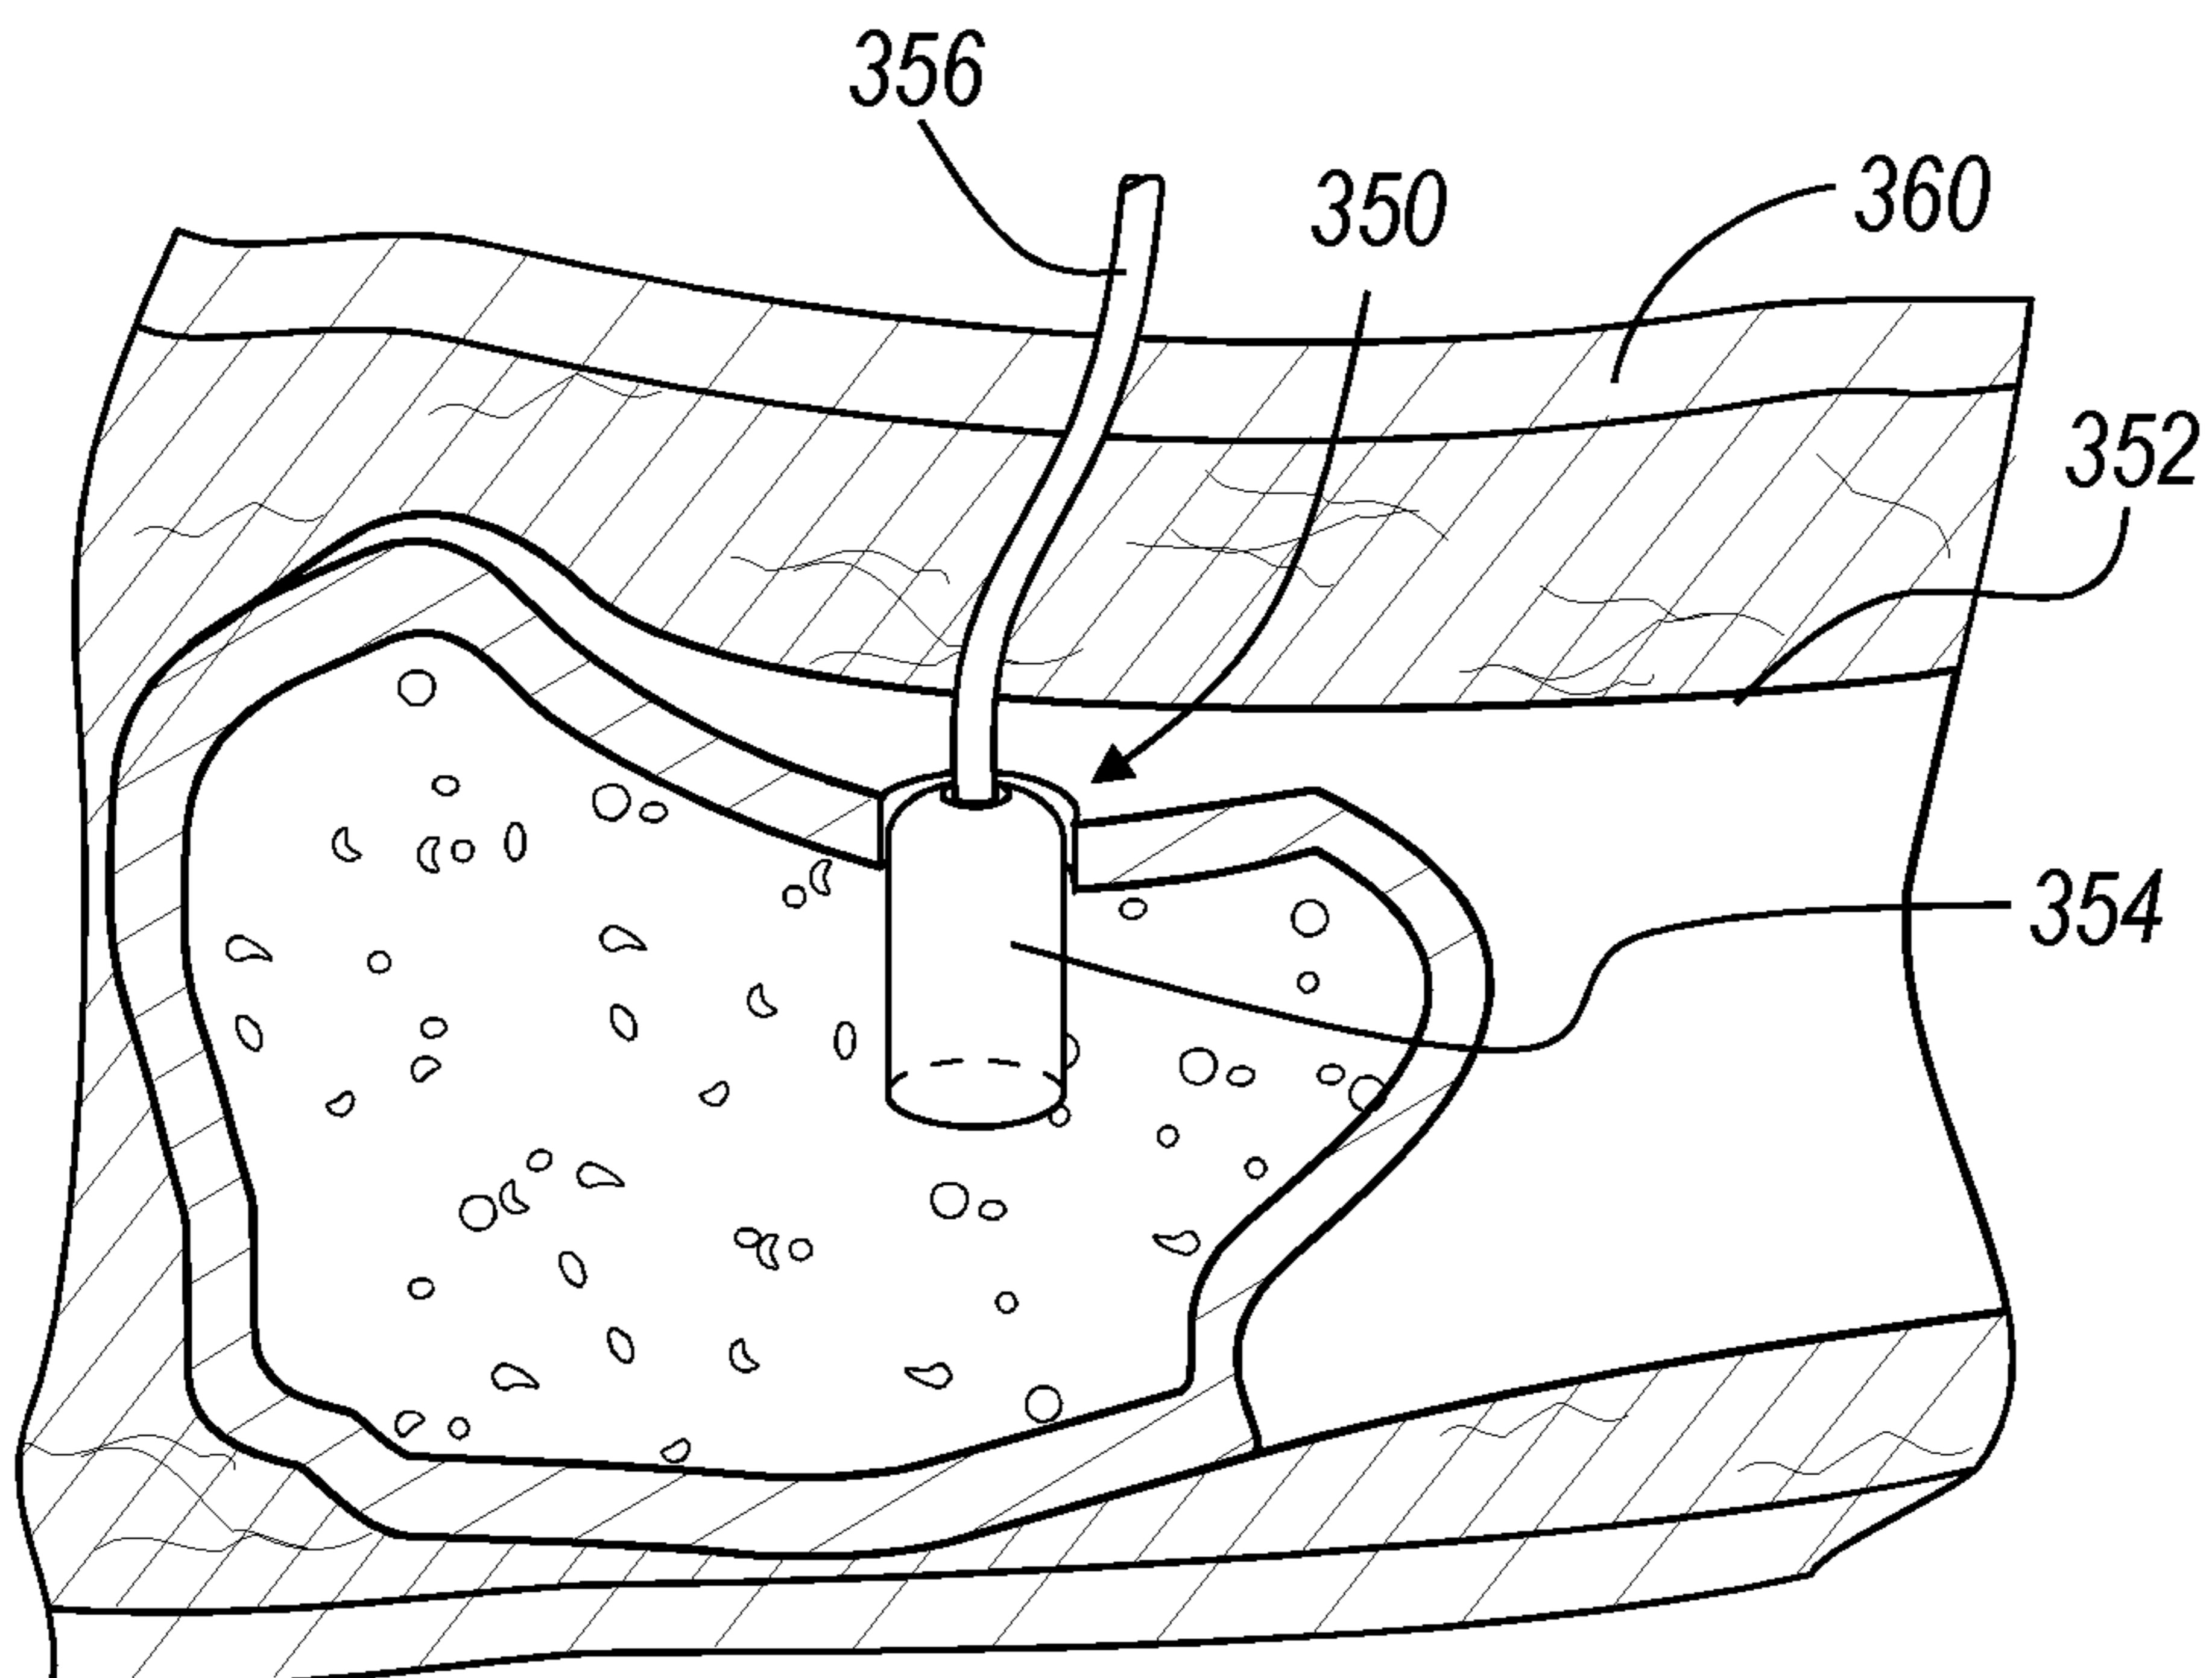


FIG. 19

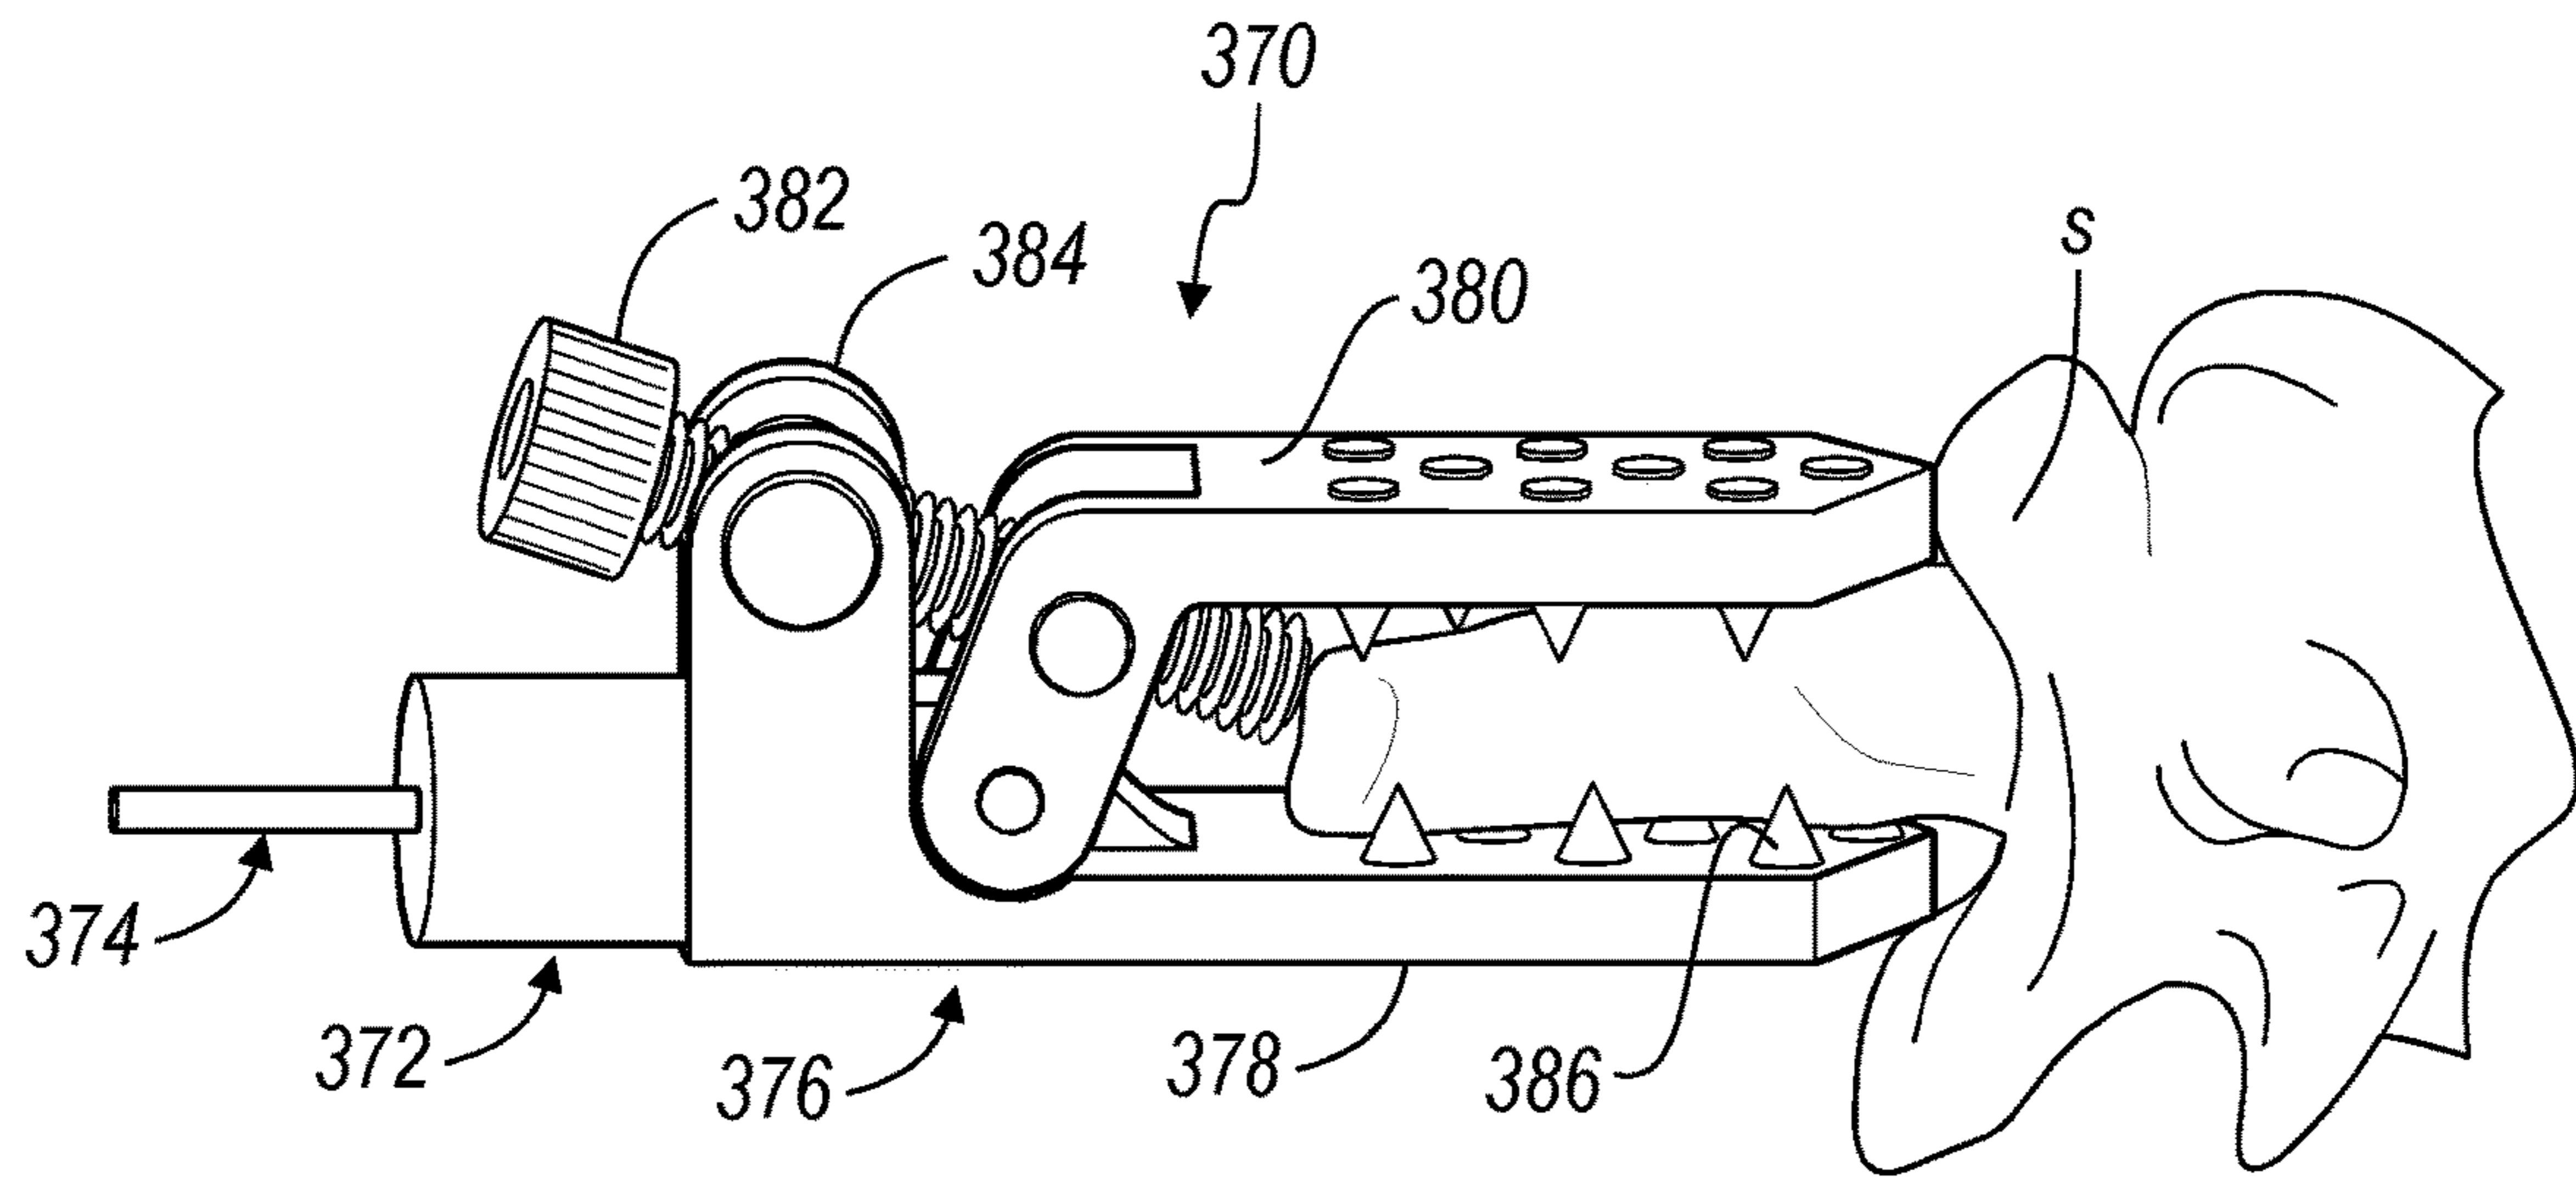


FIG. 20

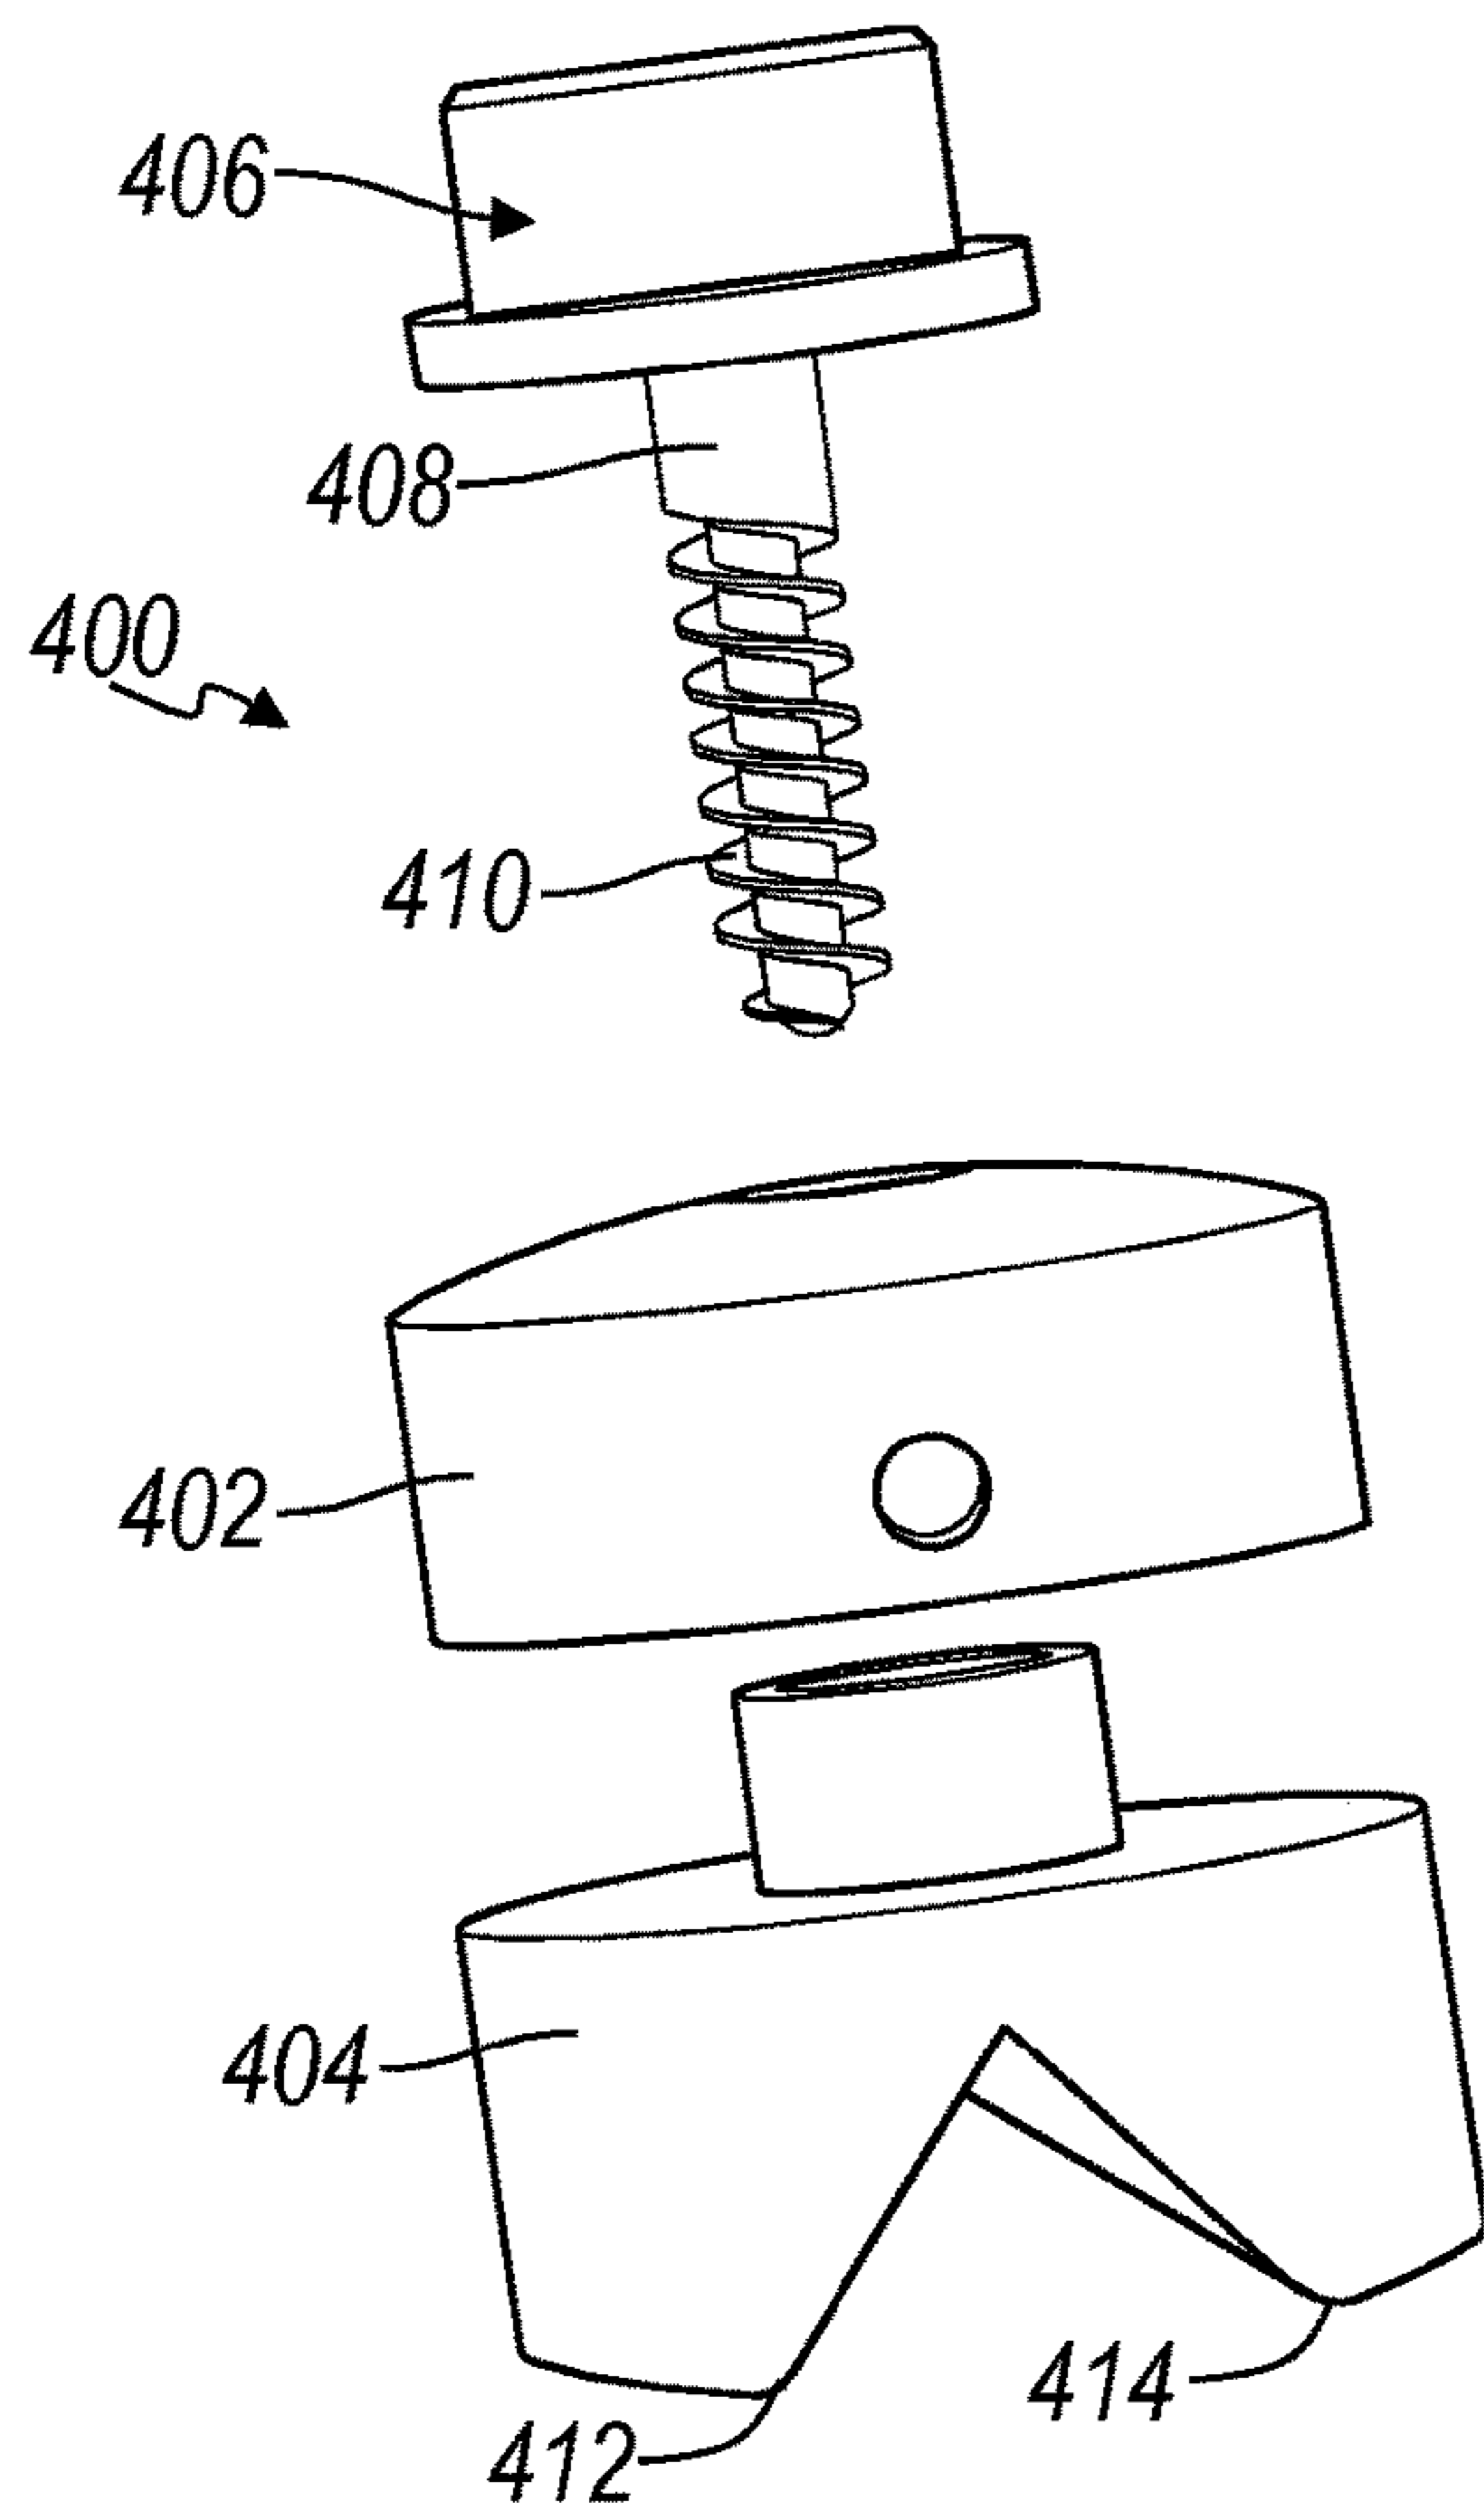


FIG. 21

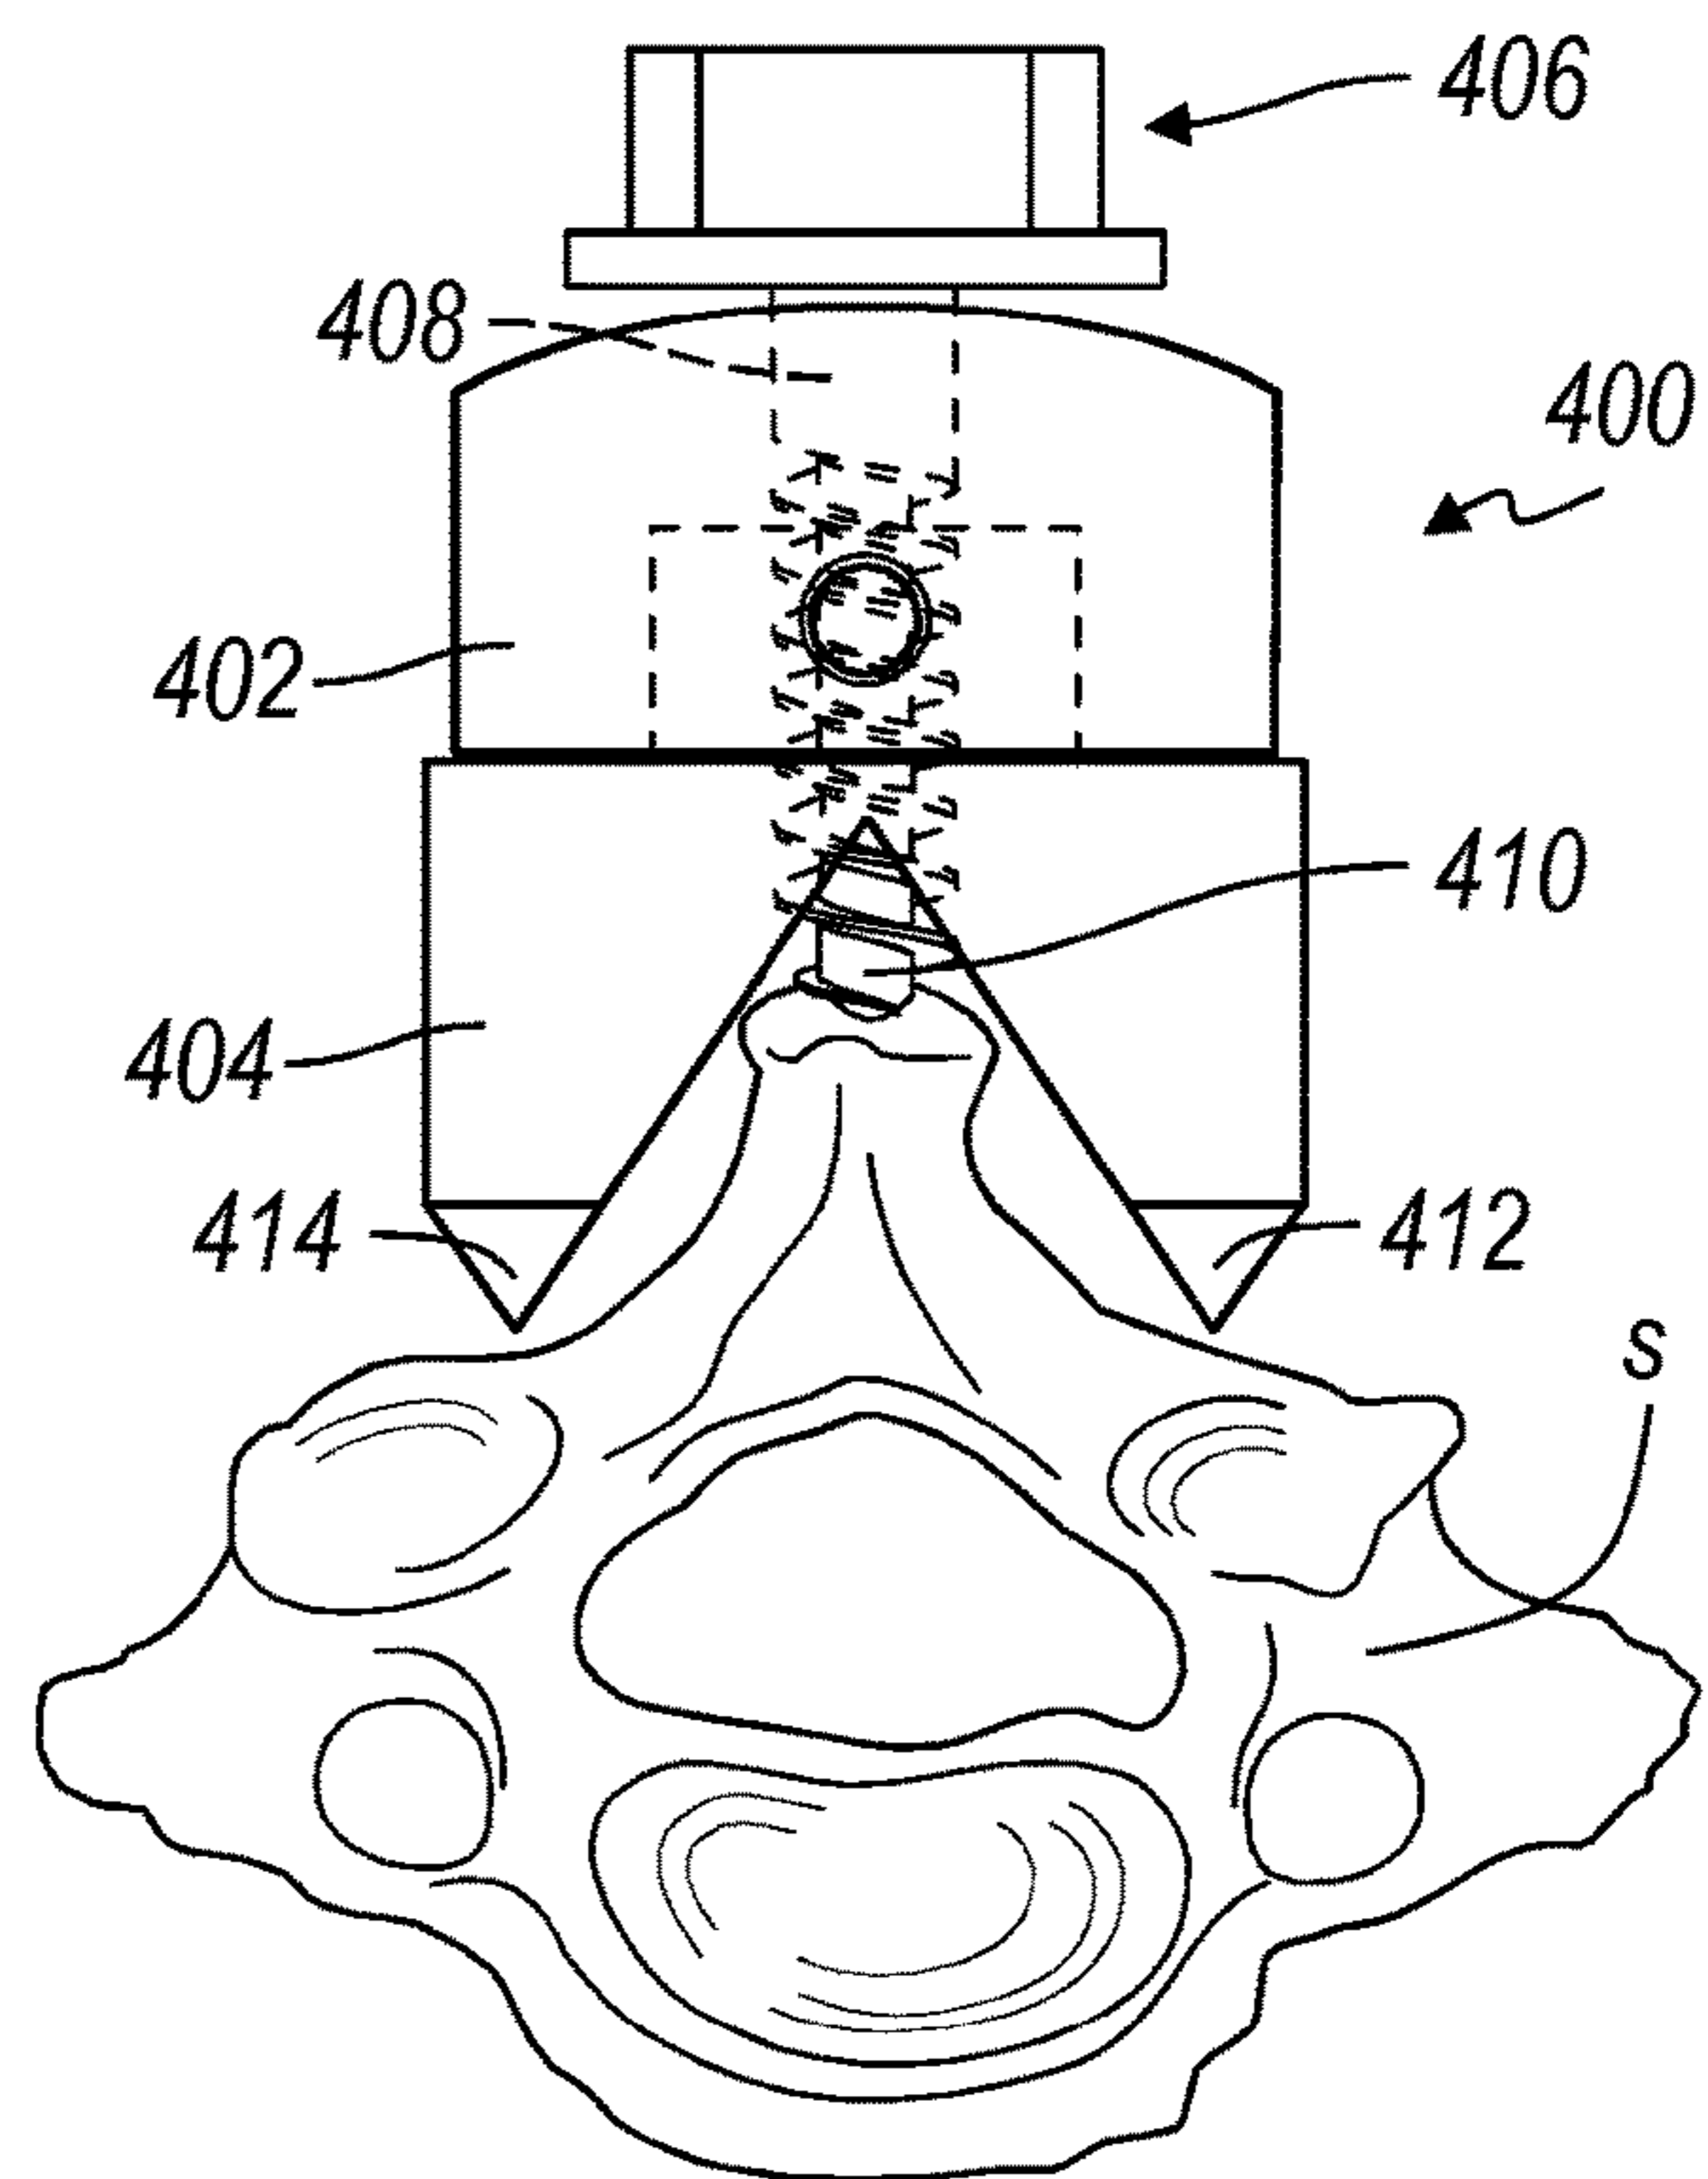


FIG. 21A

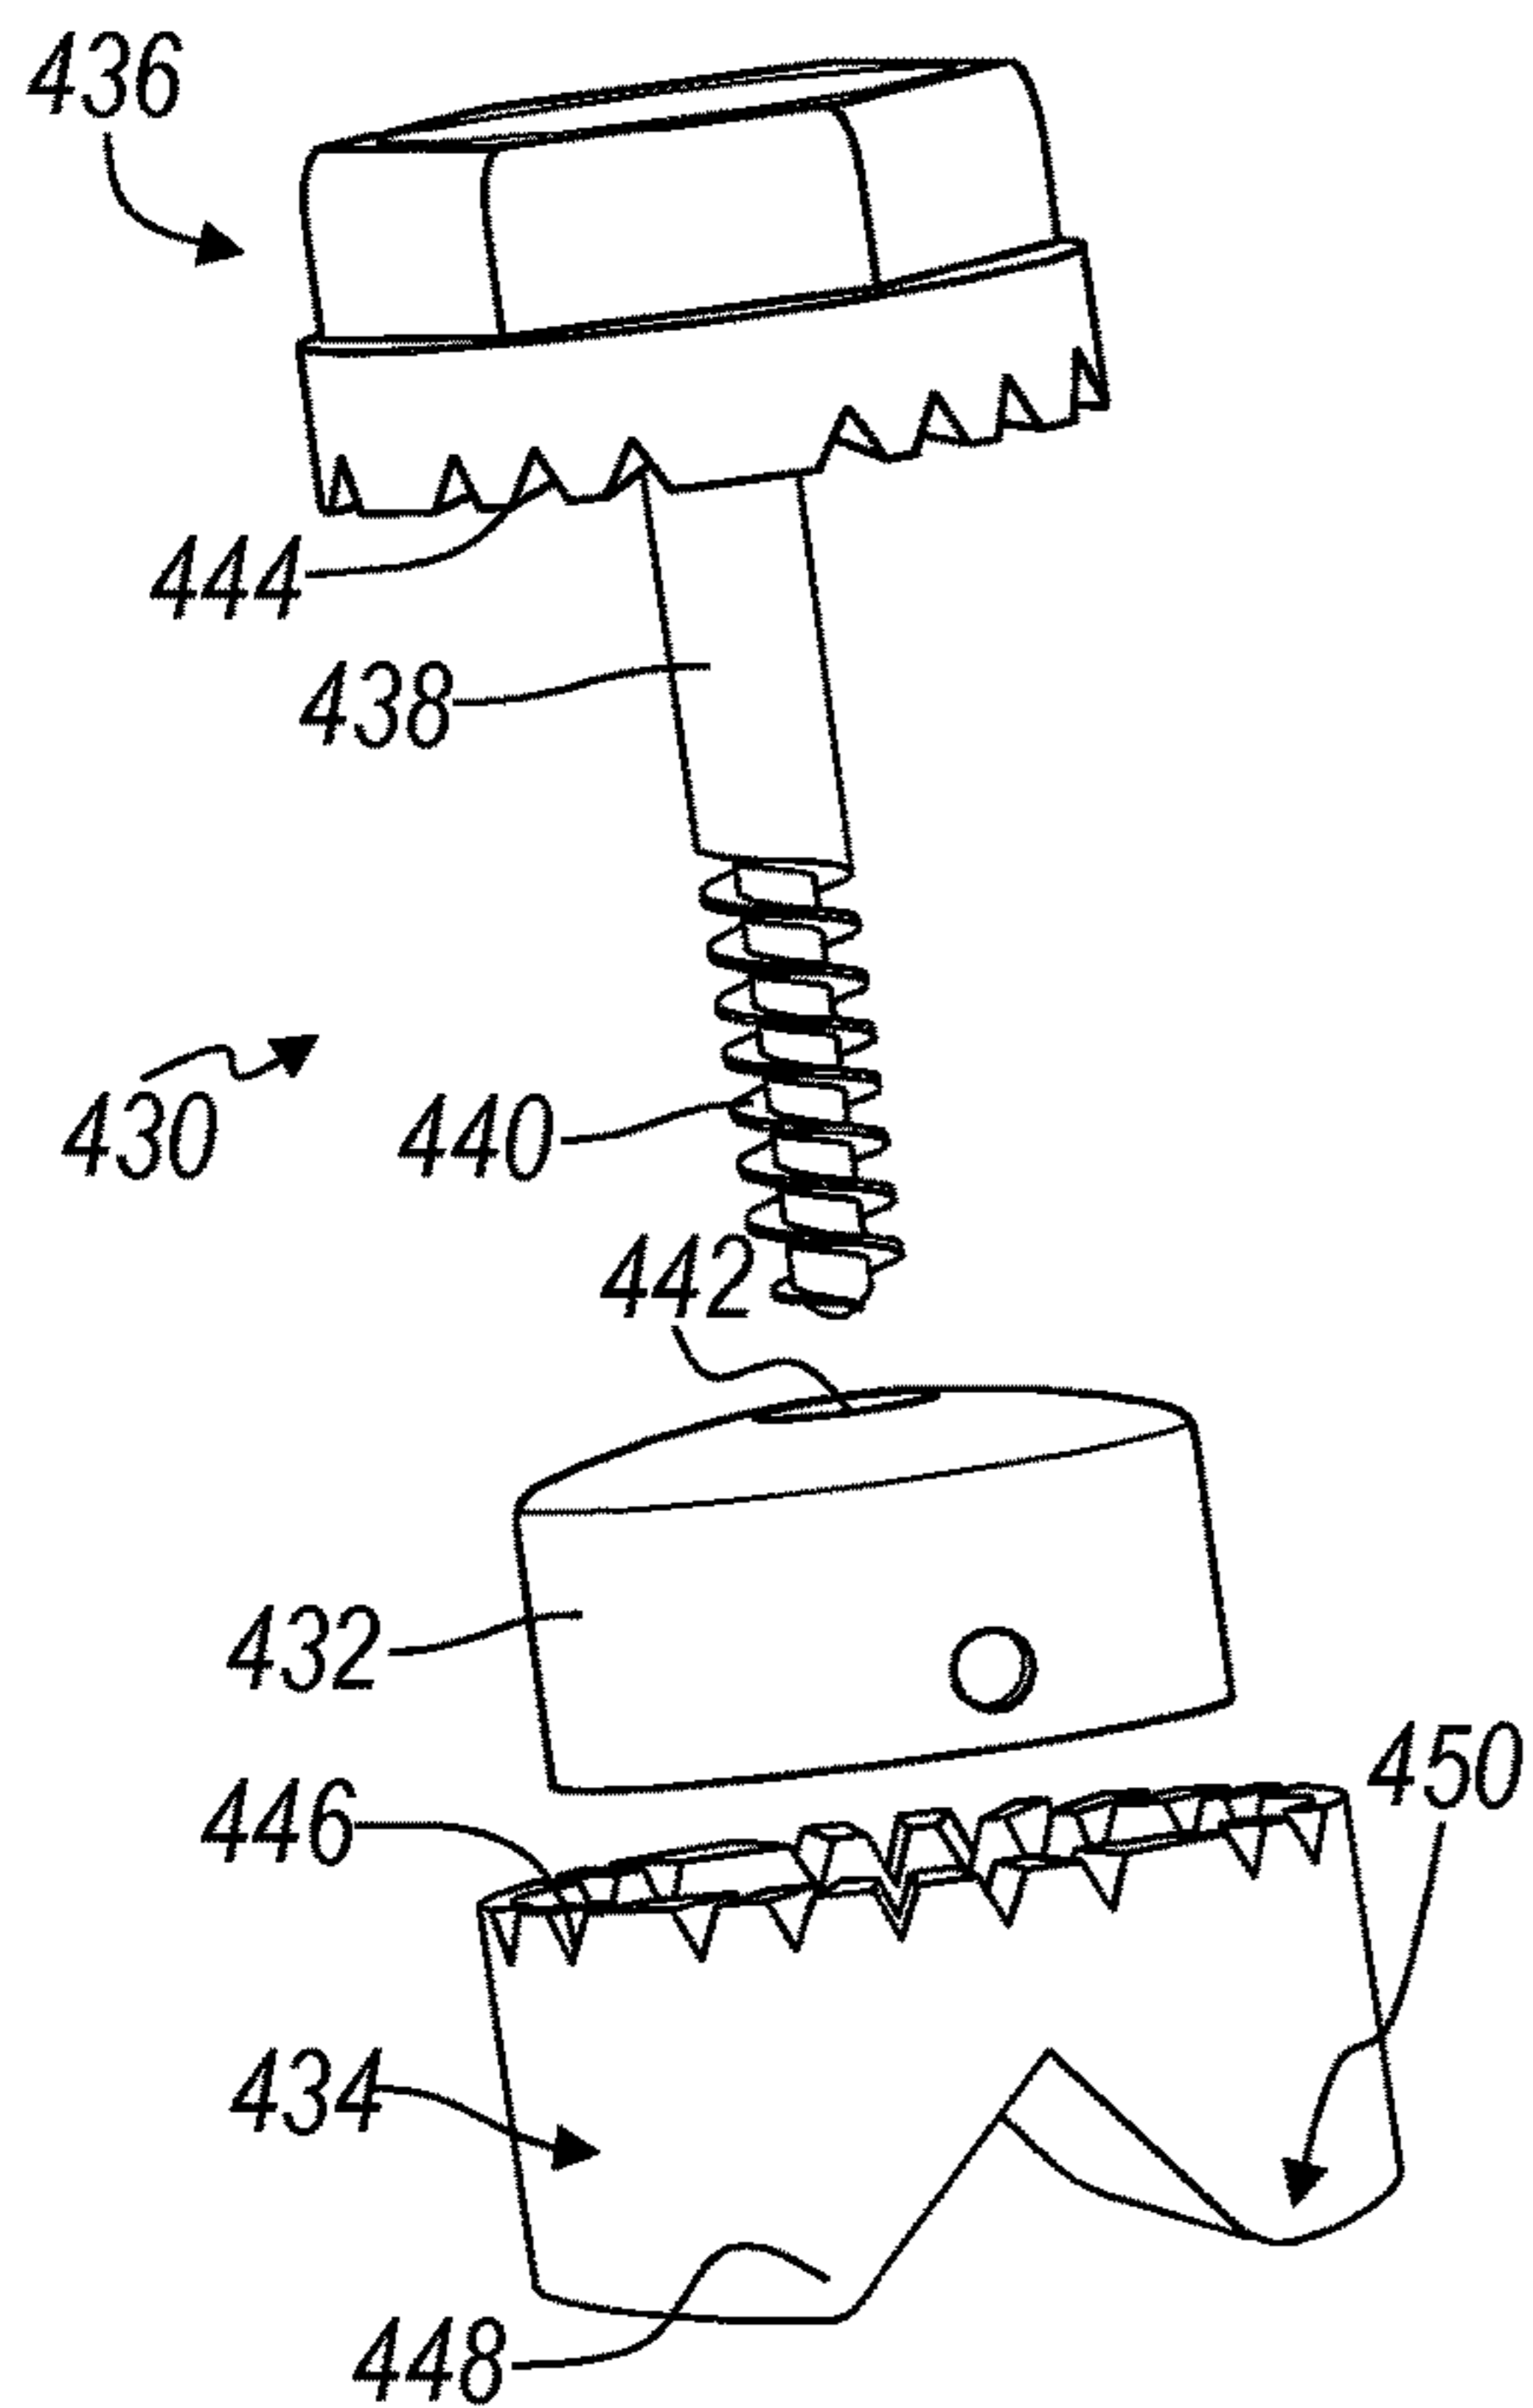


FIG. 22

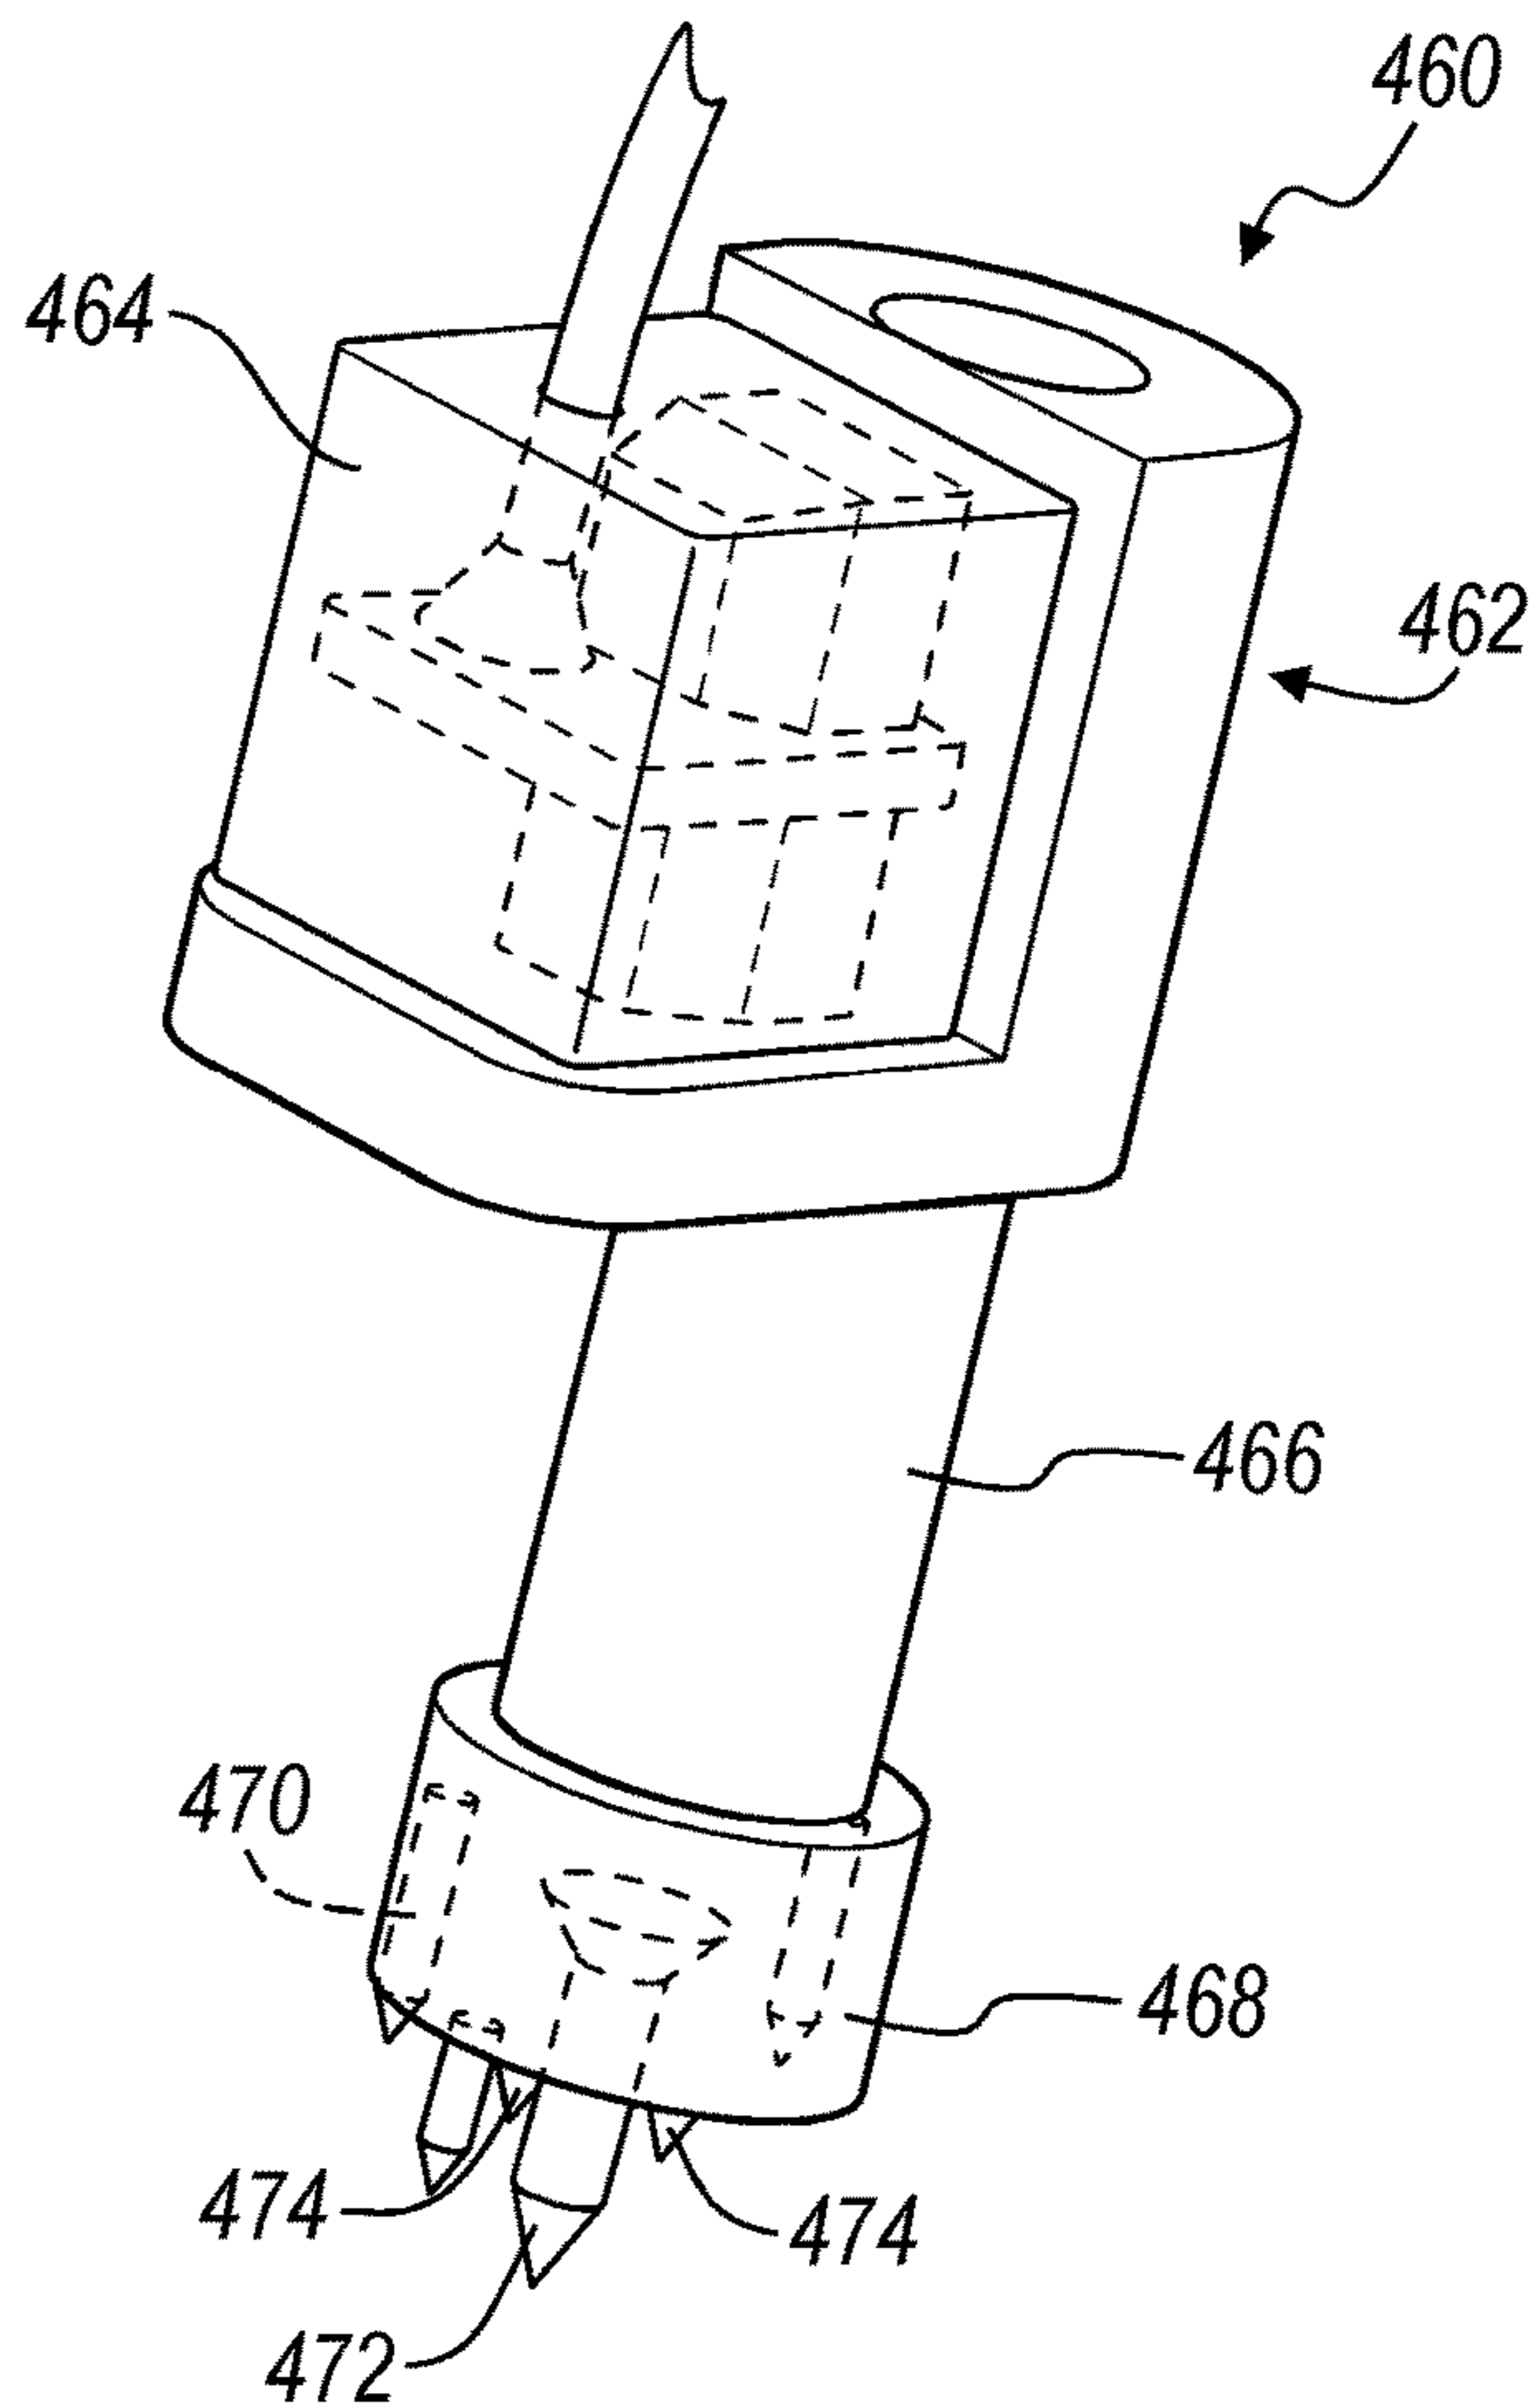


FIG. 23

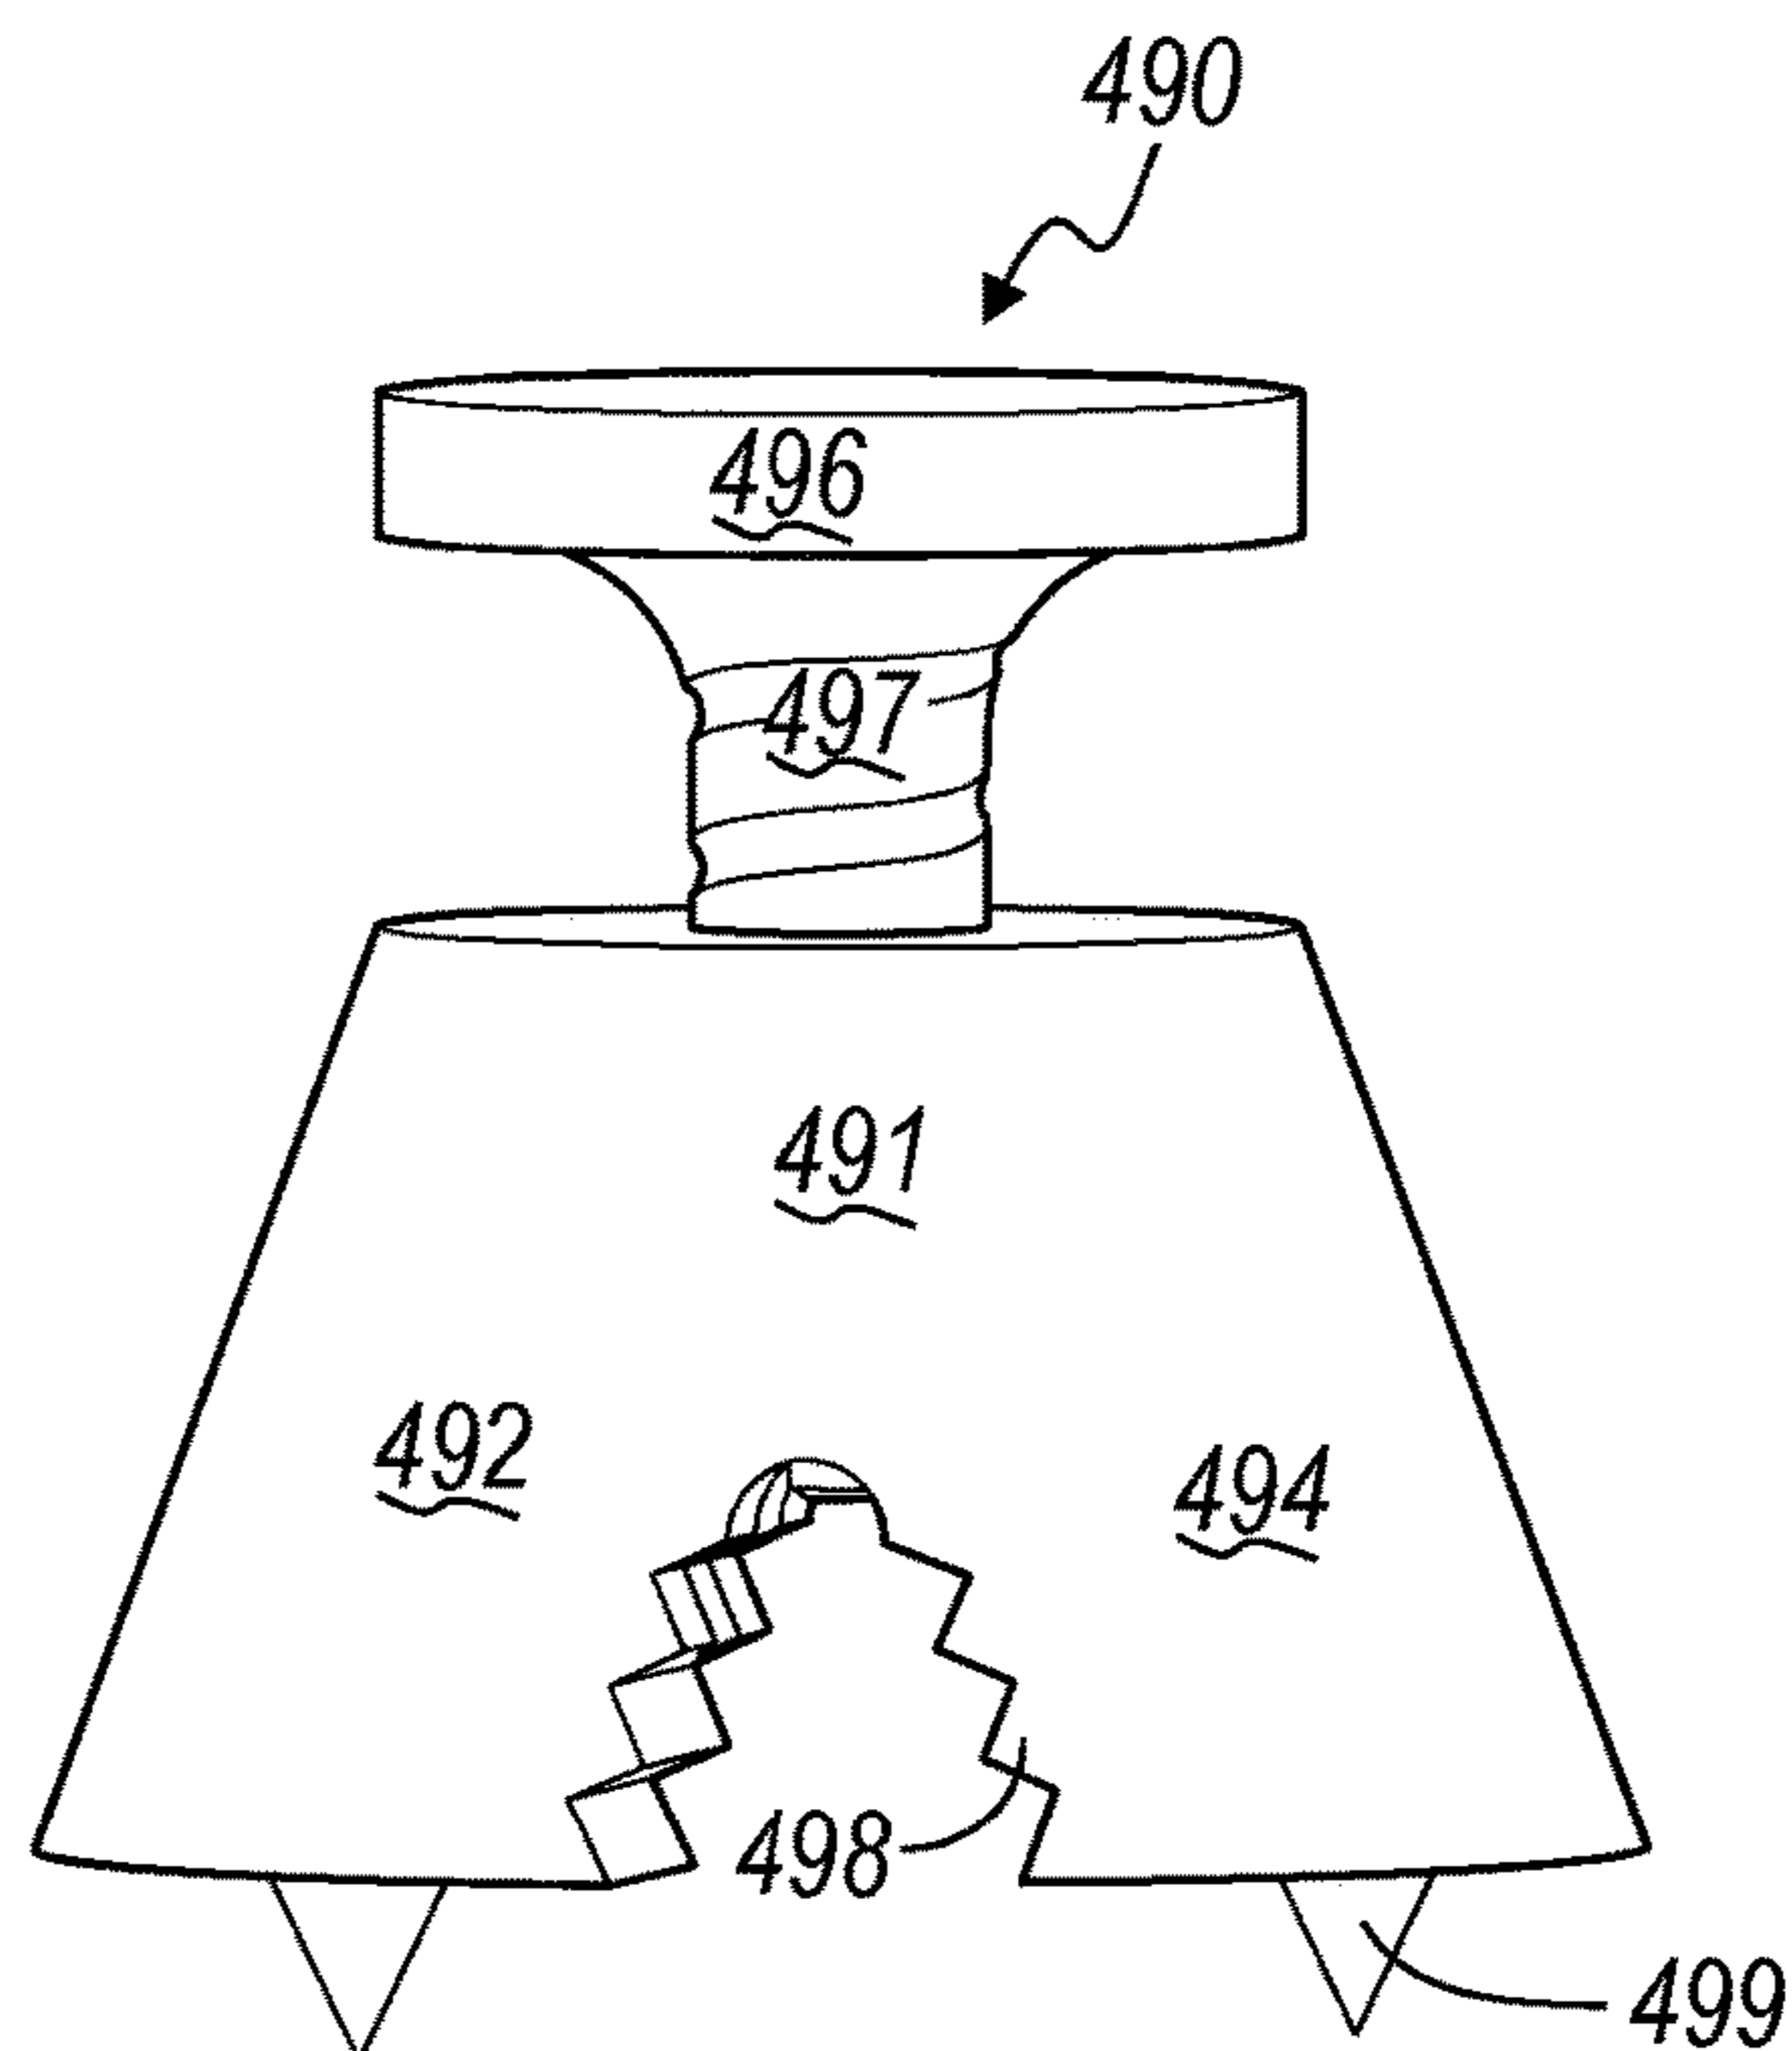
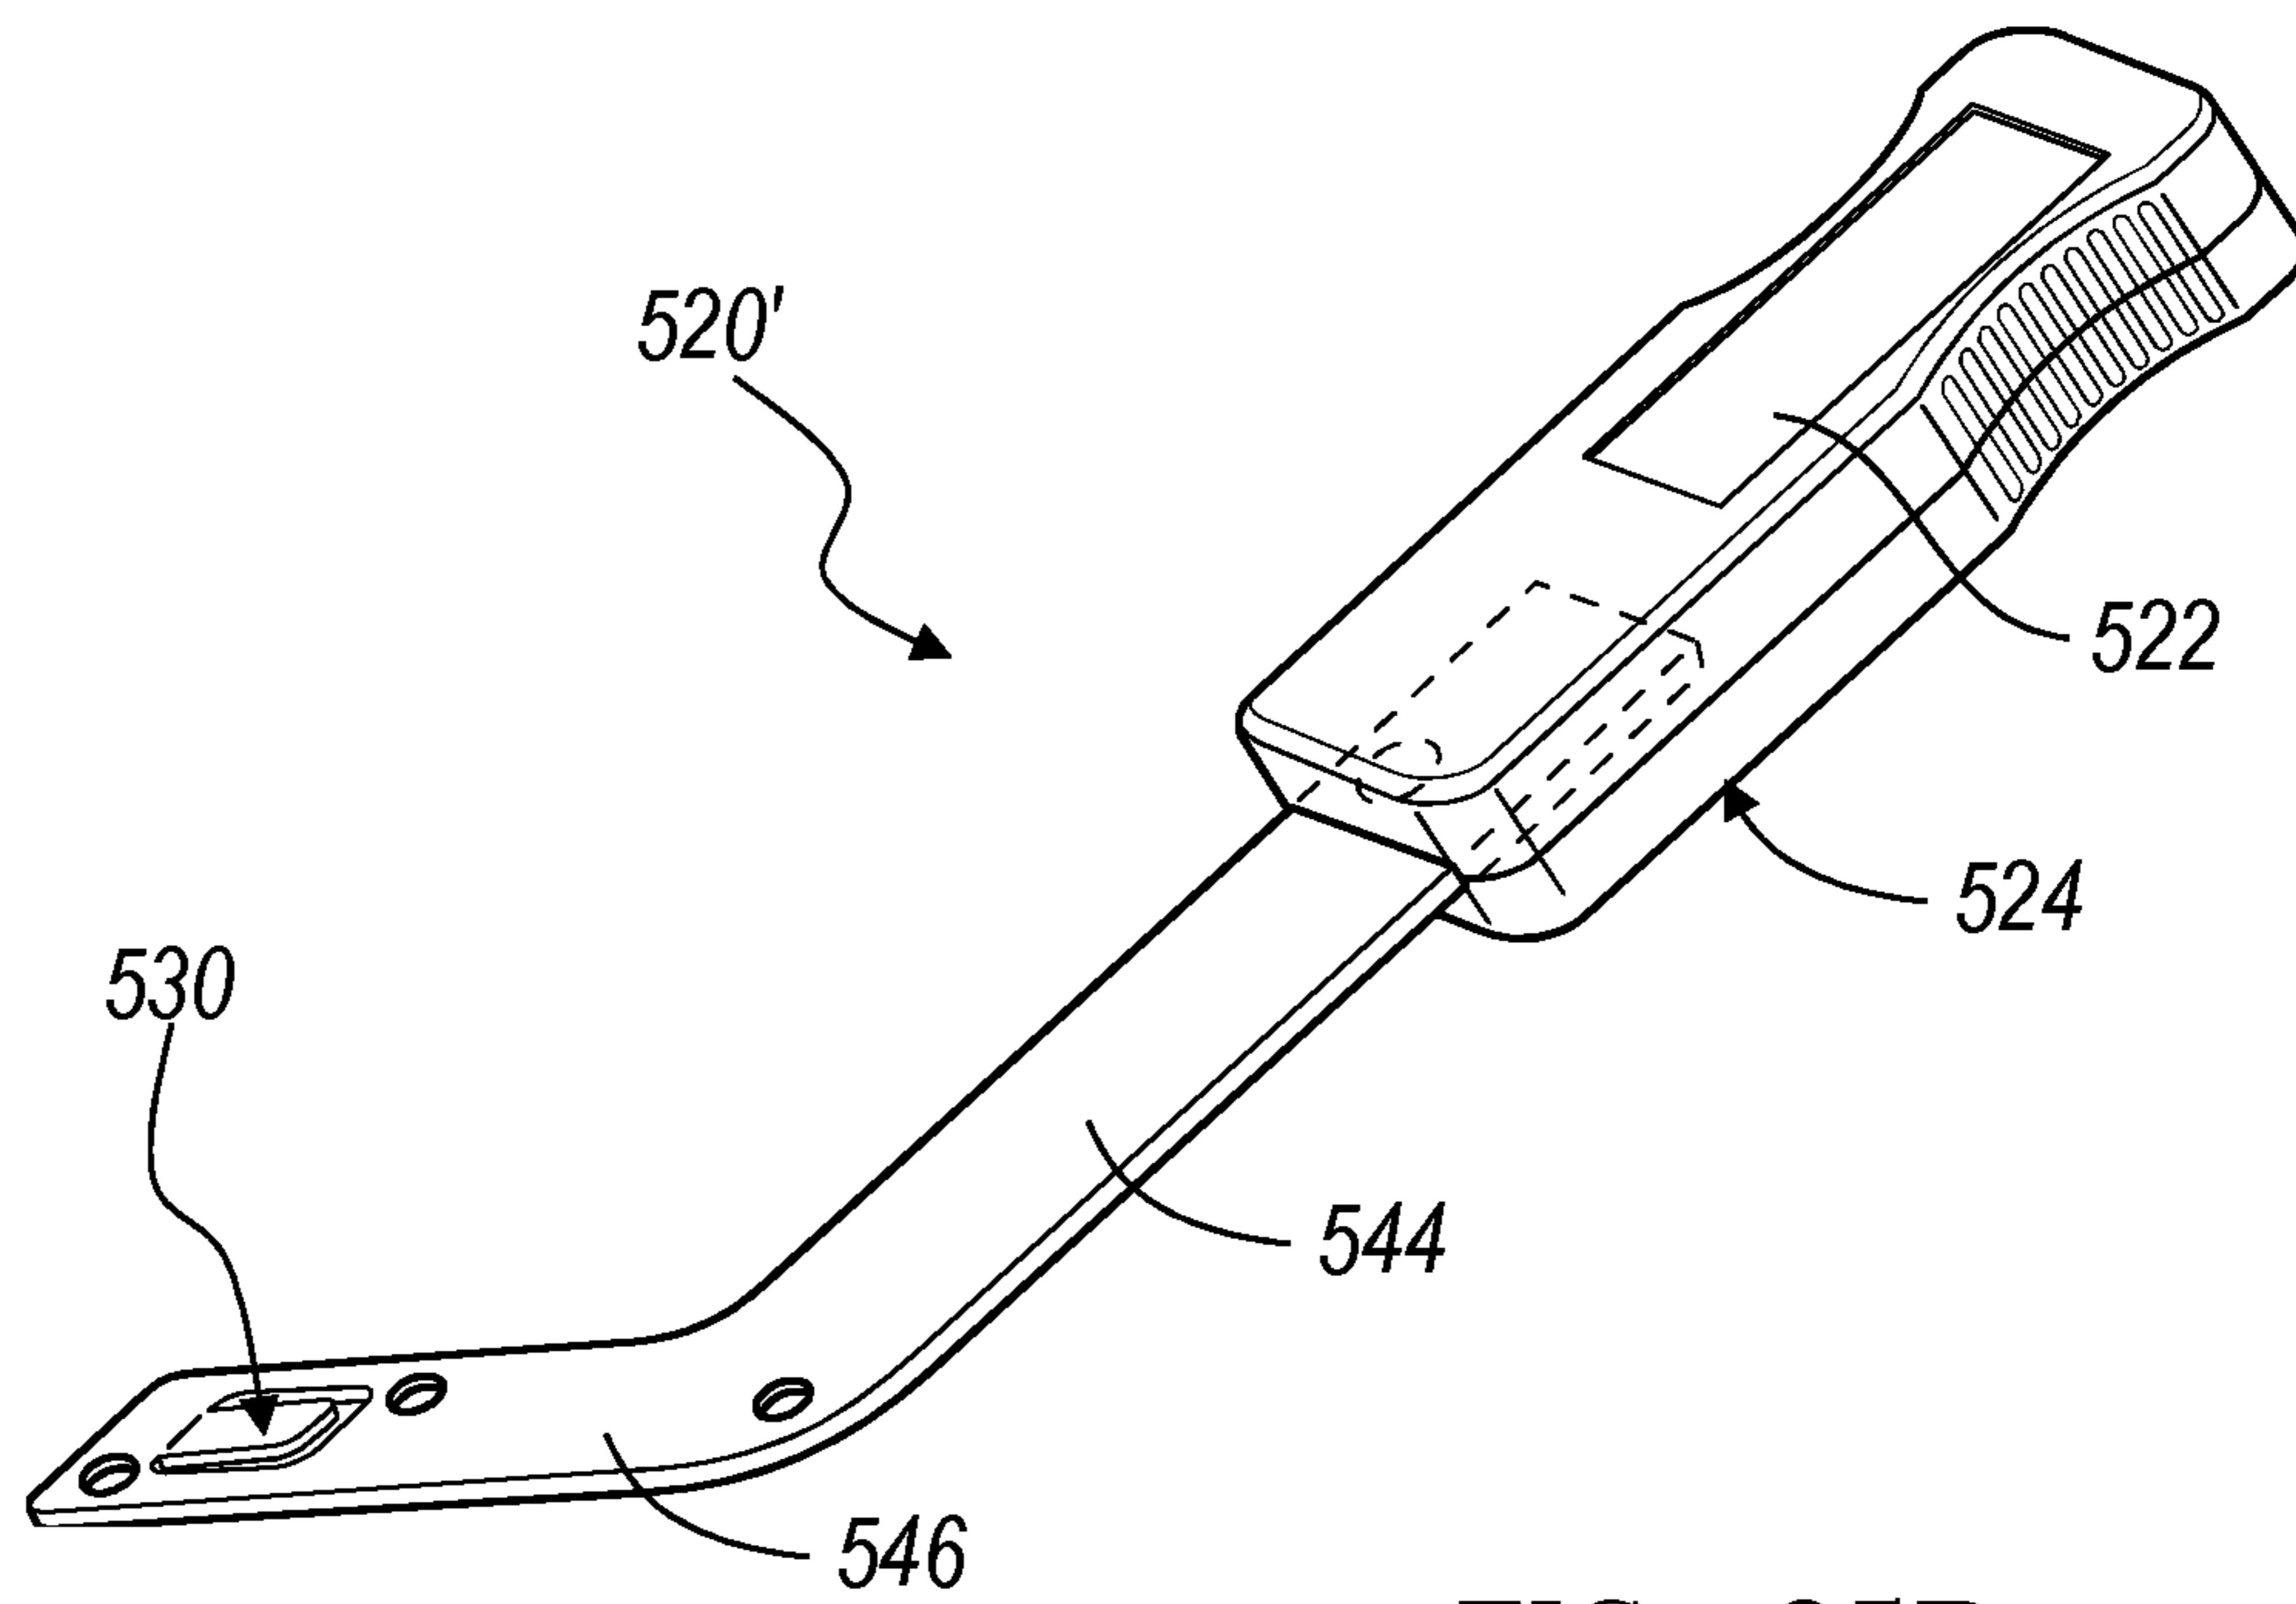
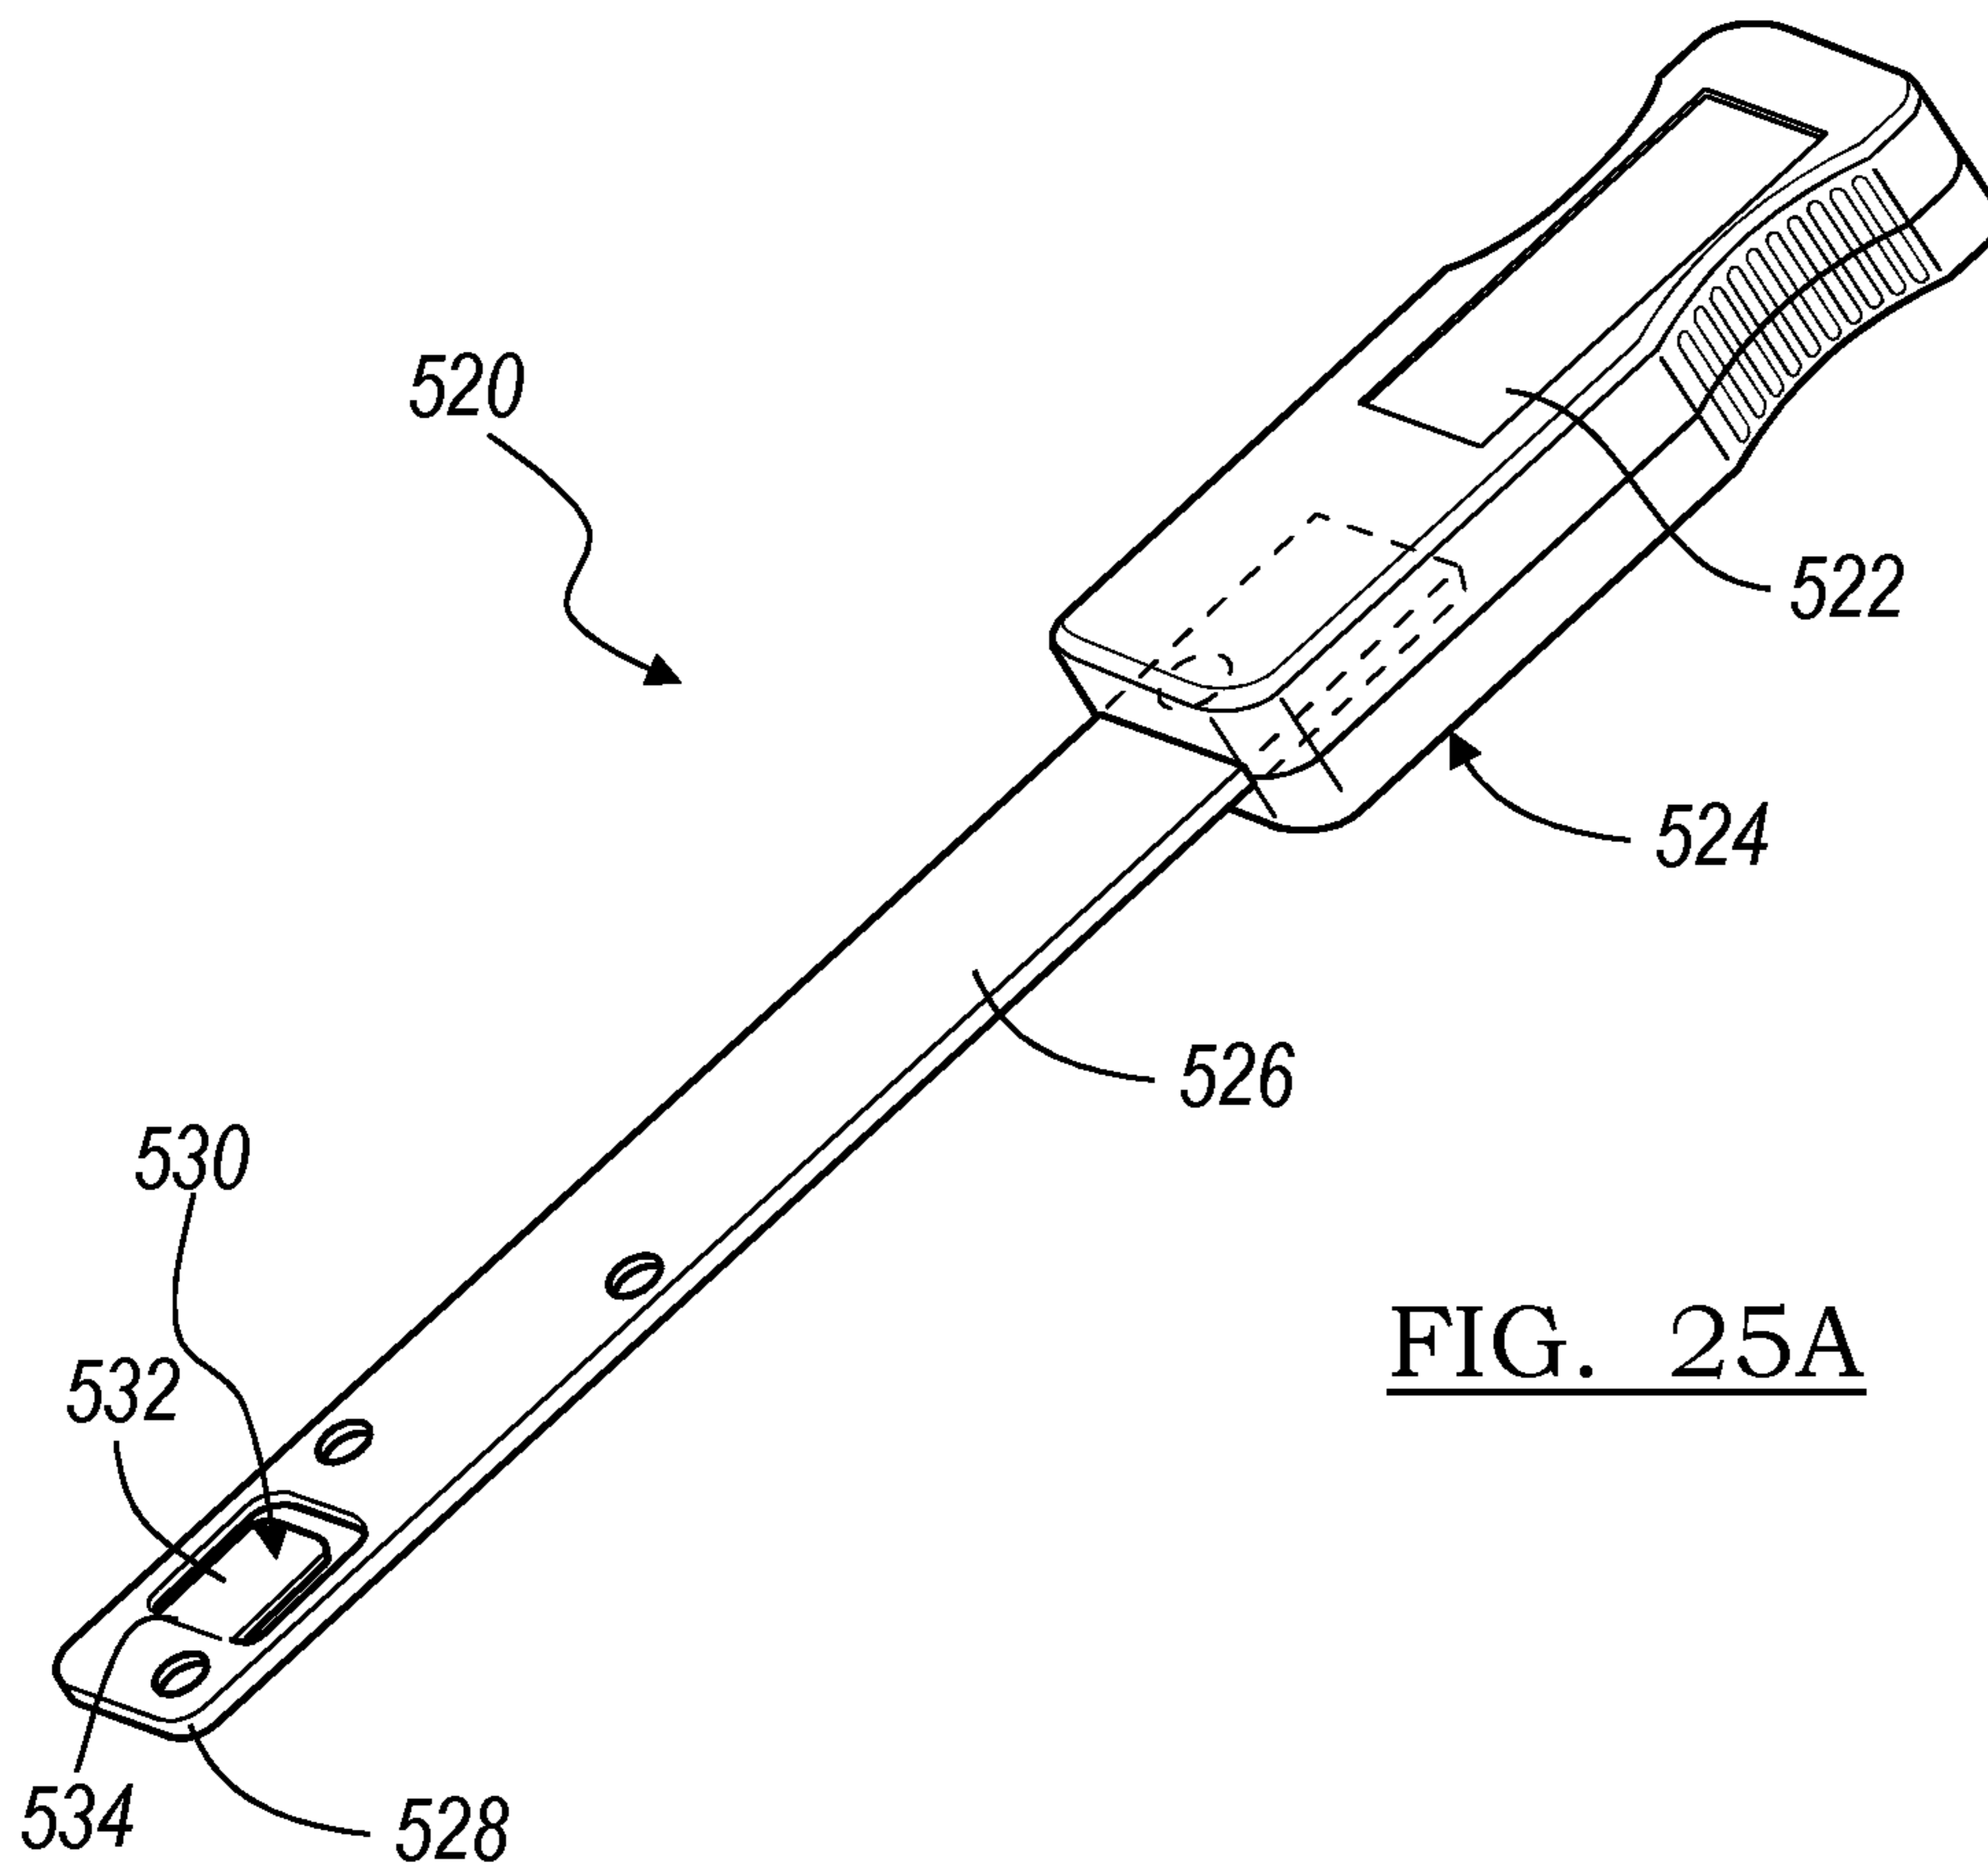
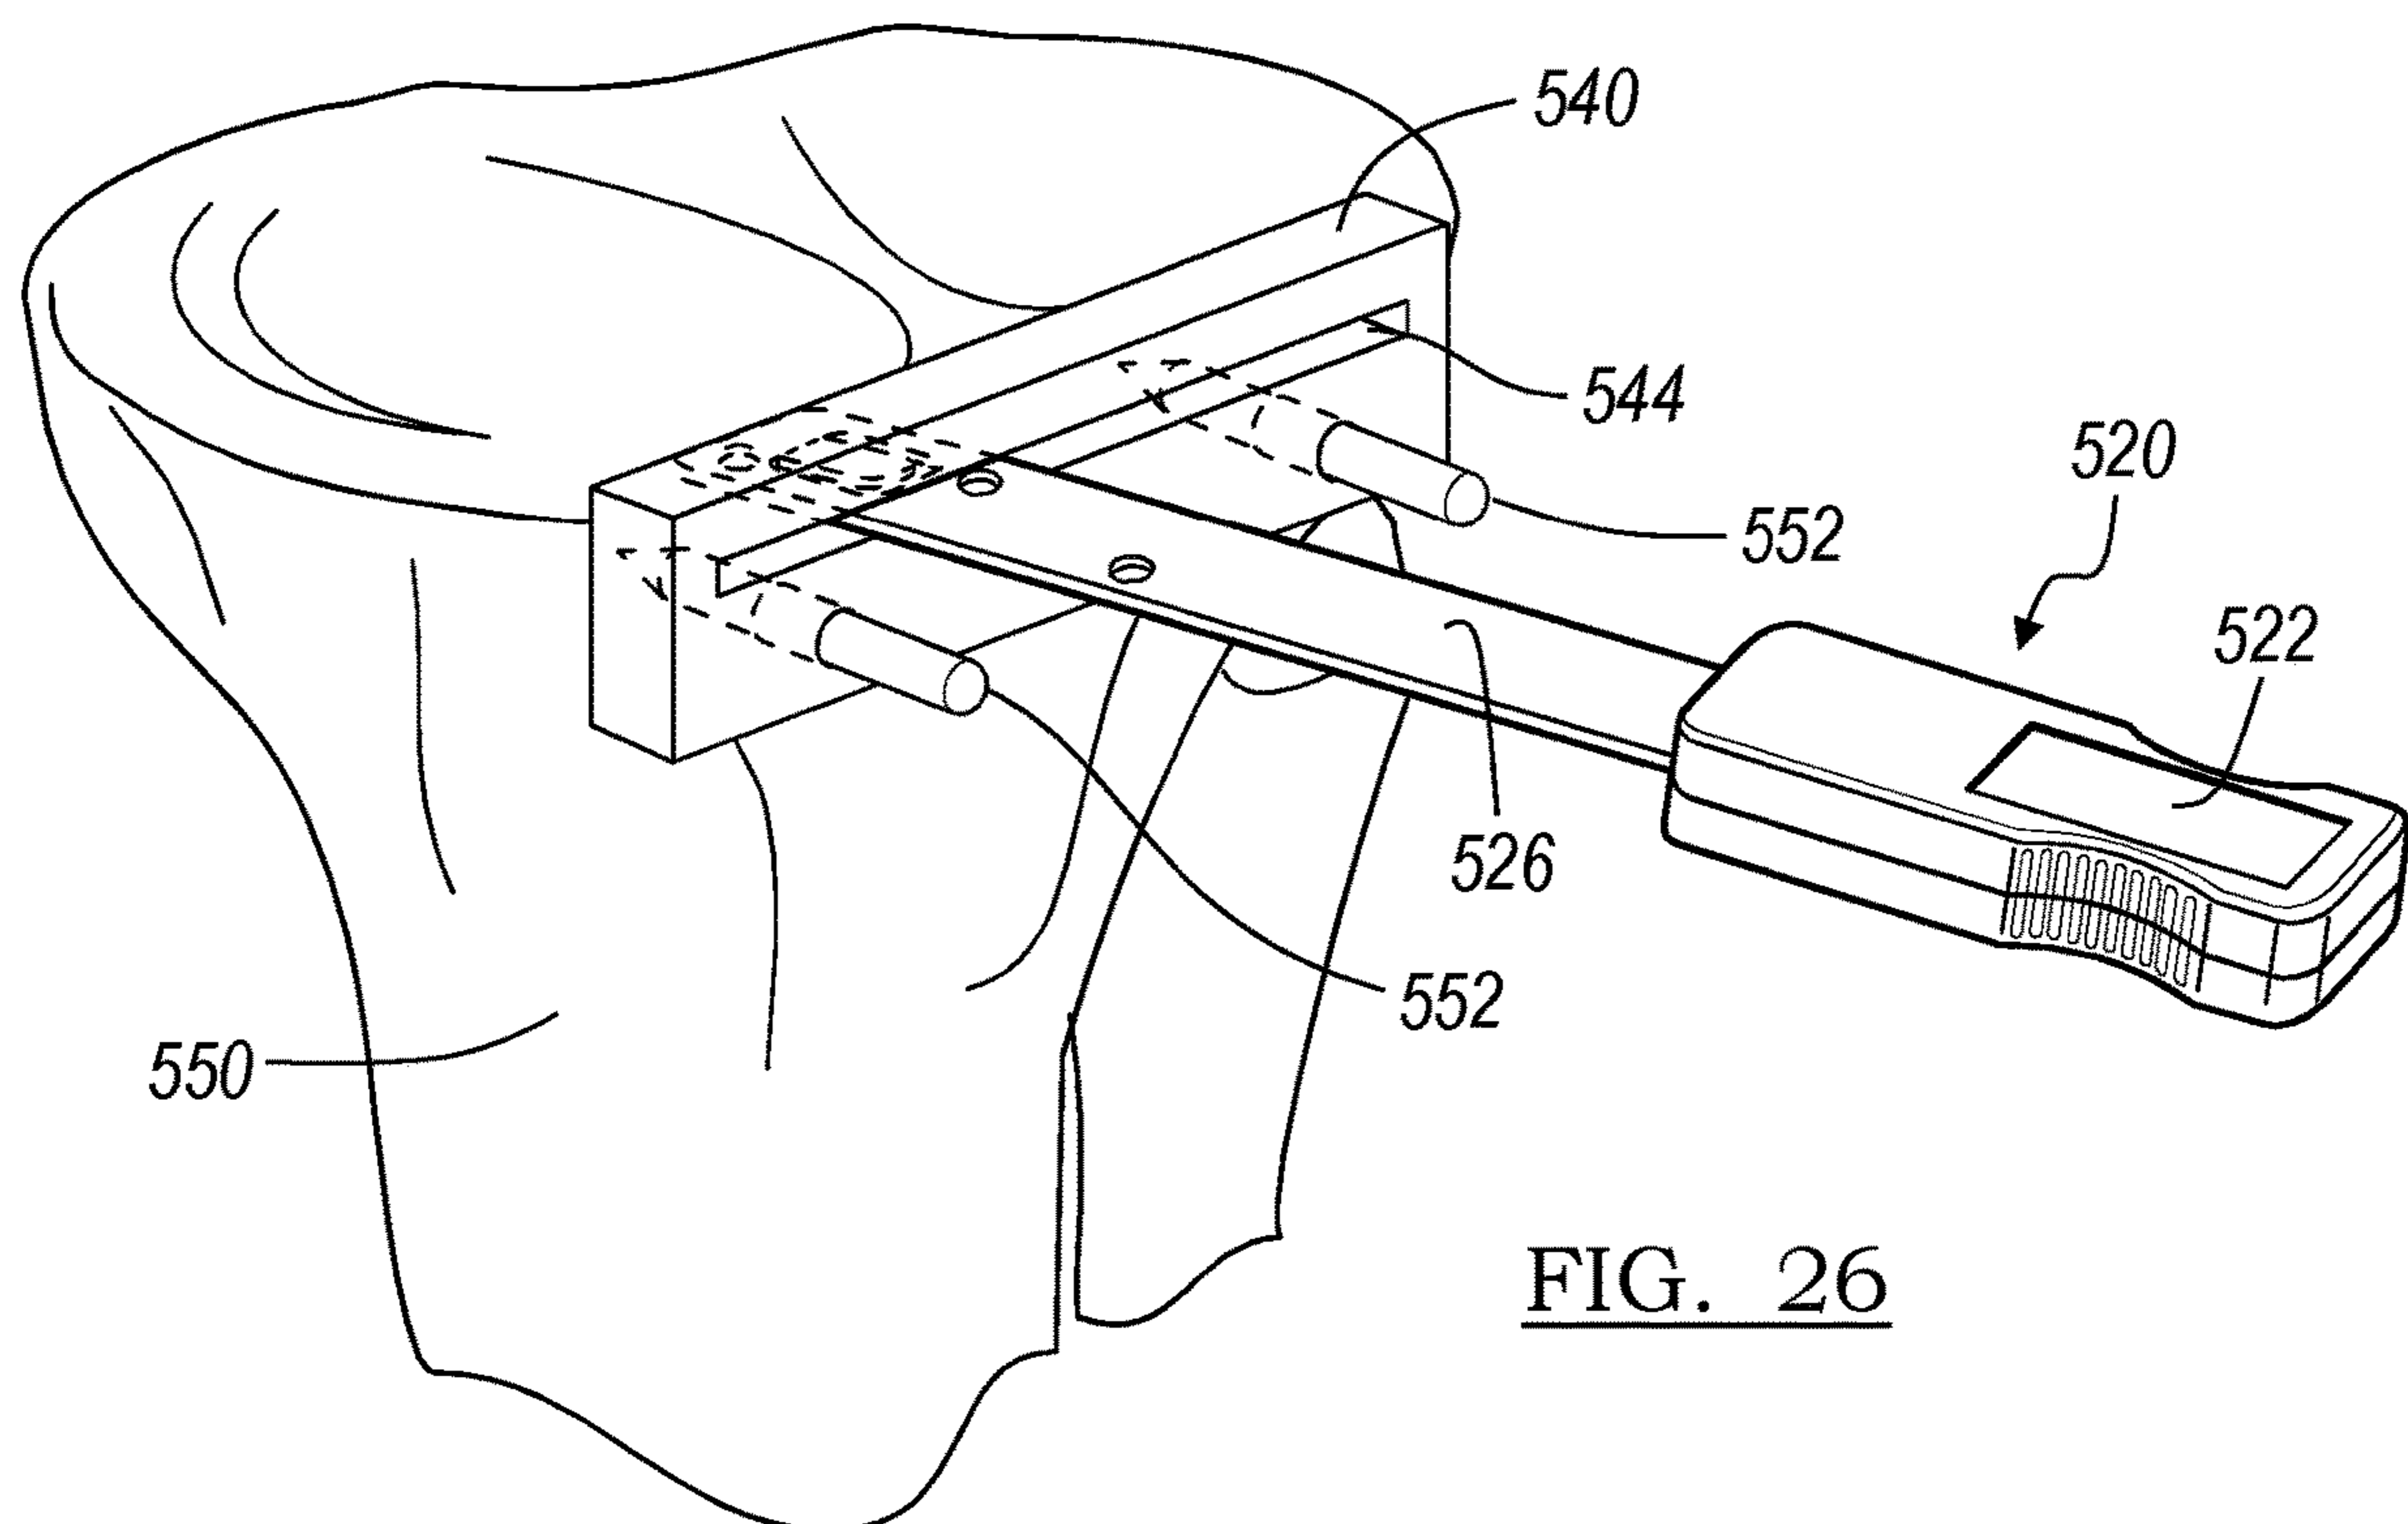


FIG. 24





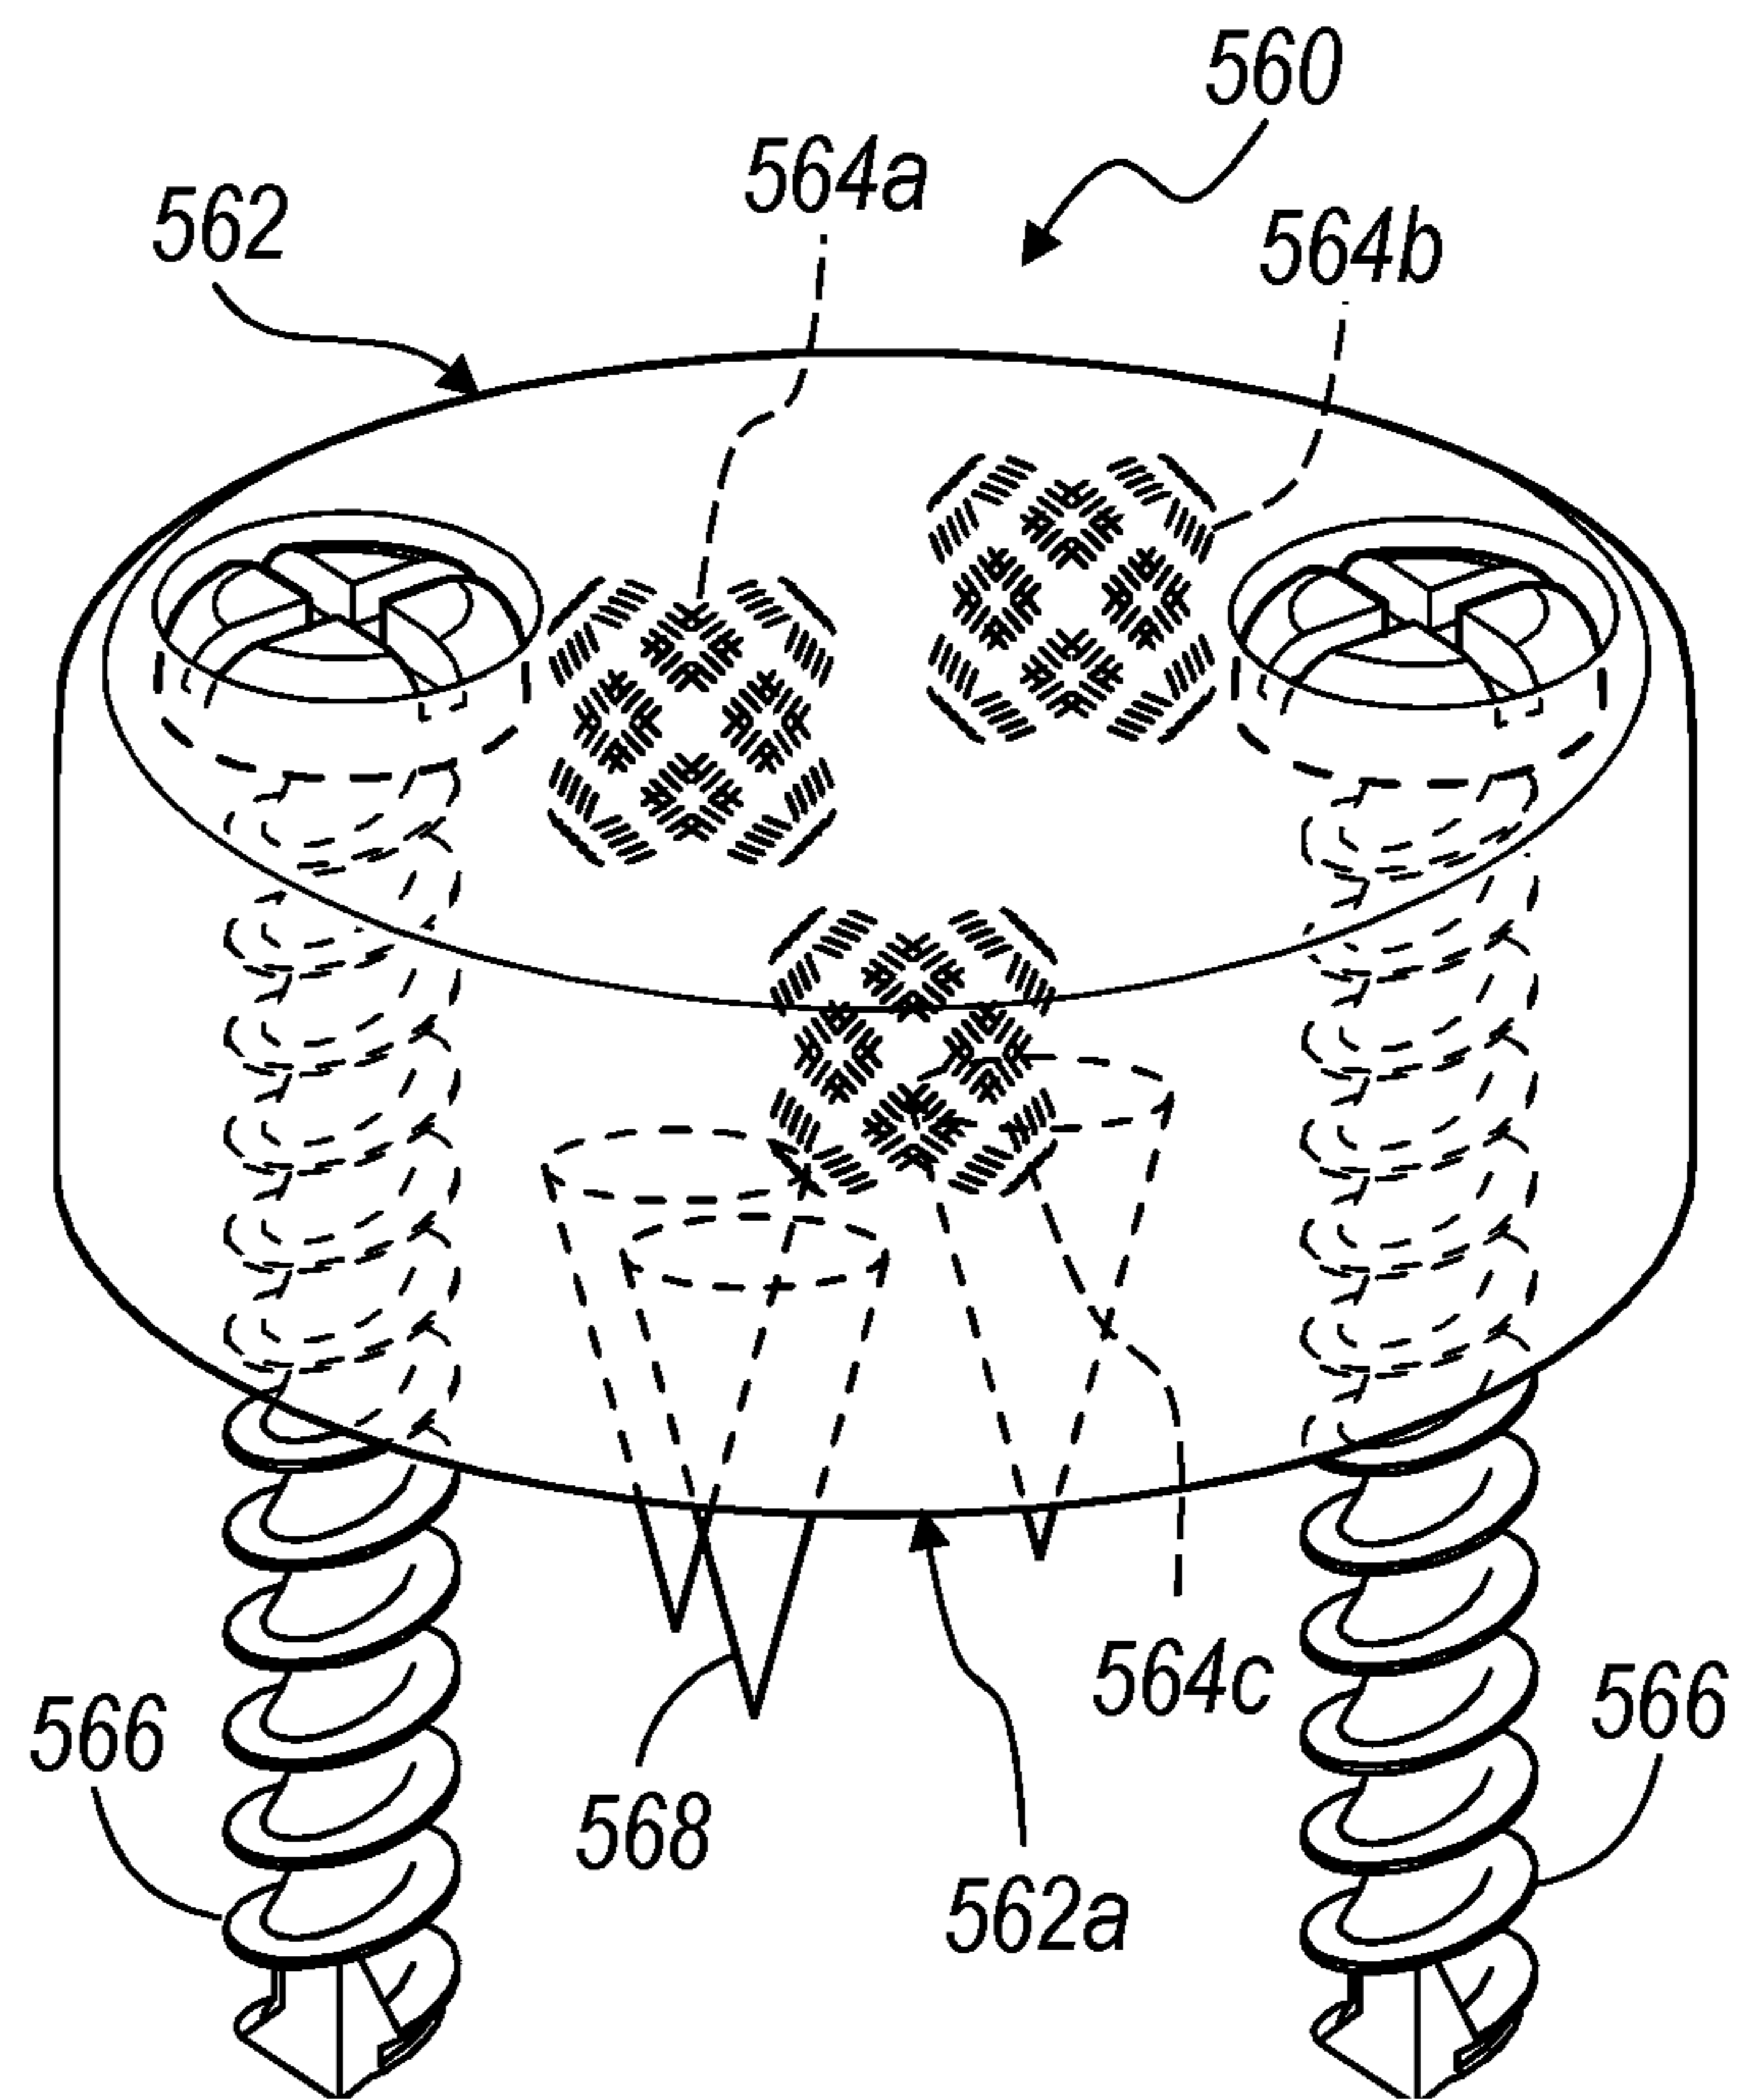


FIG. 27A

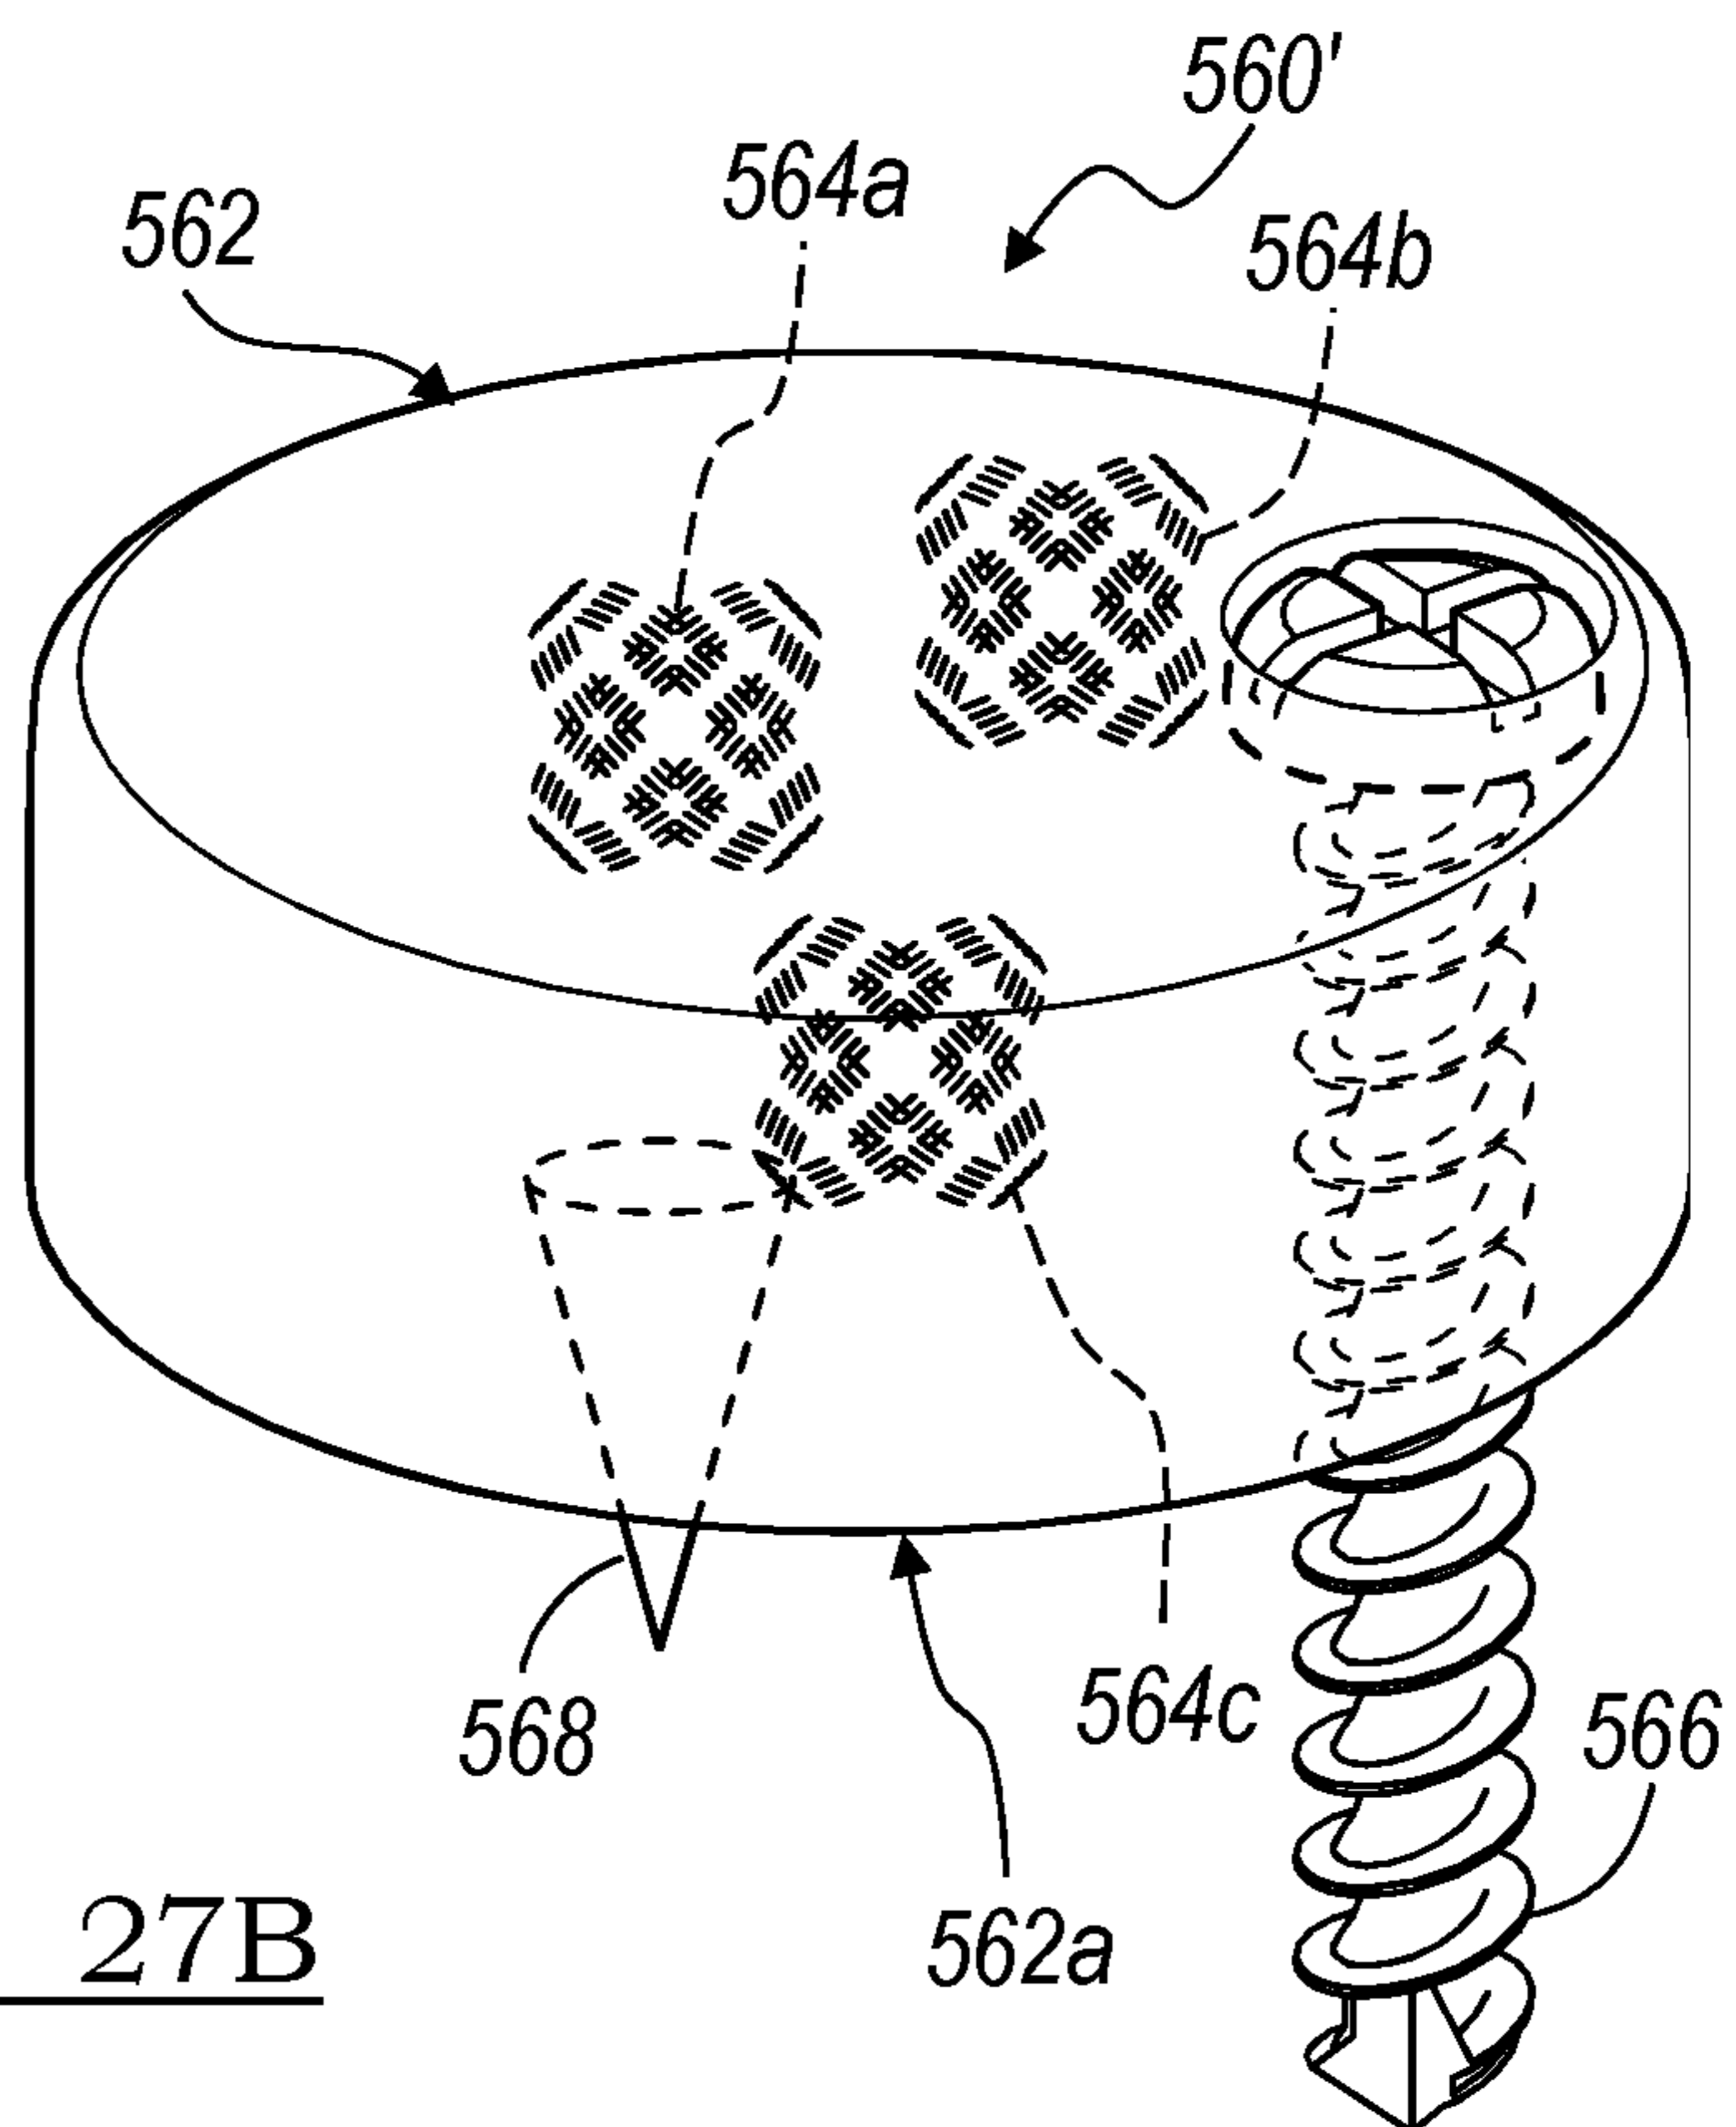


FIG. 27B

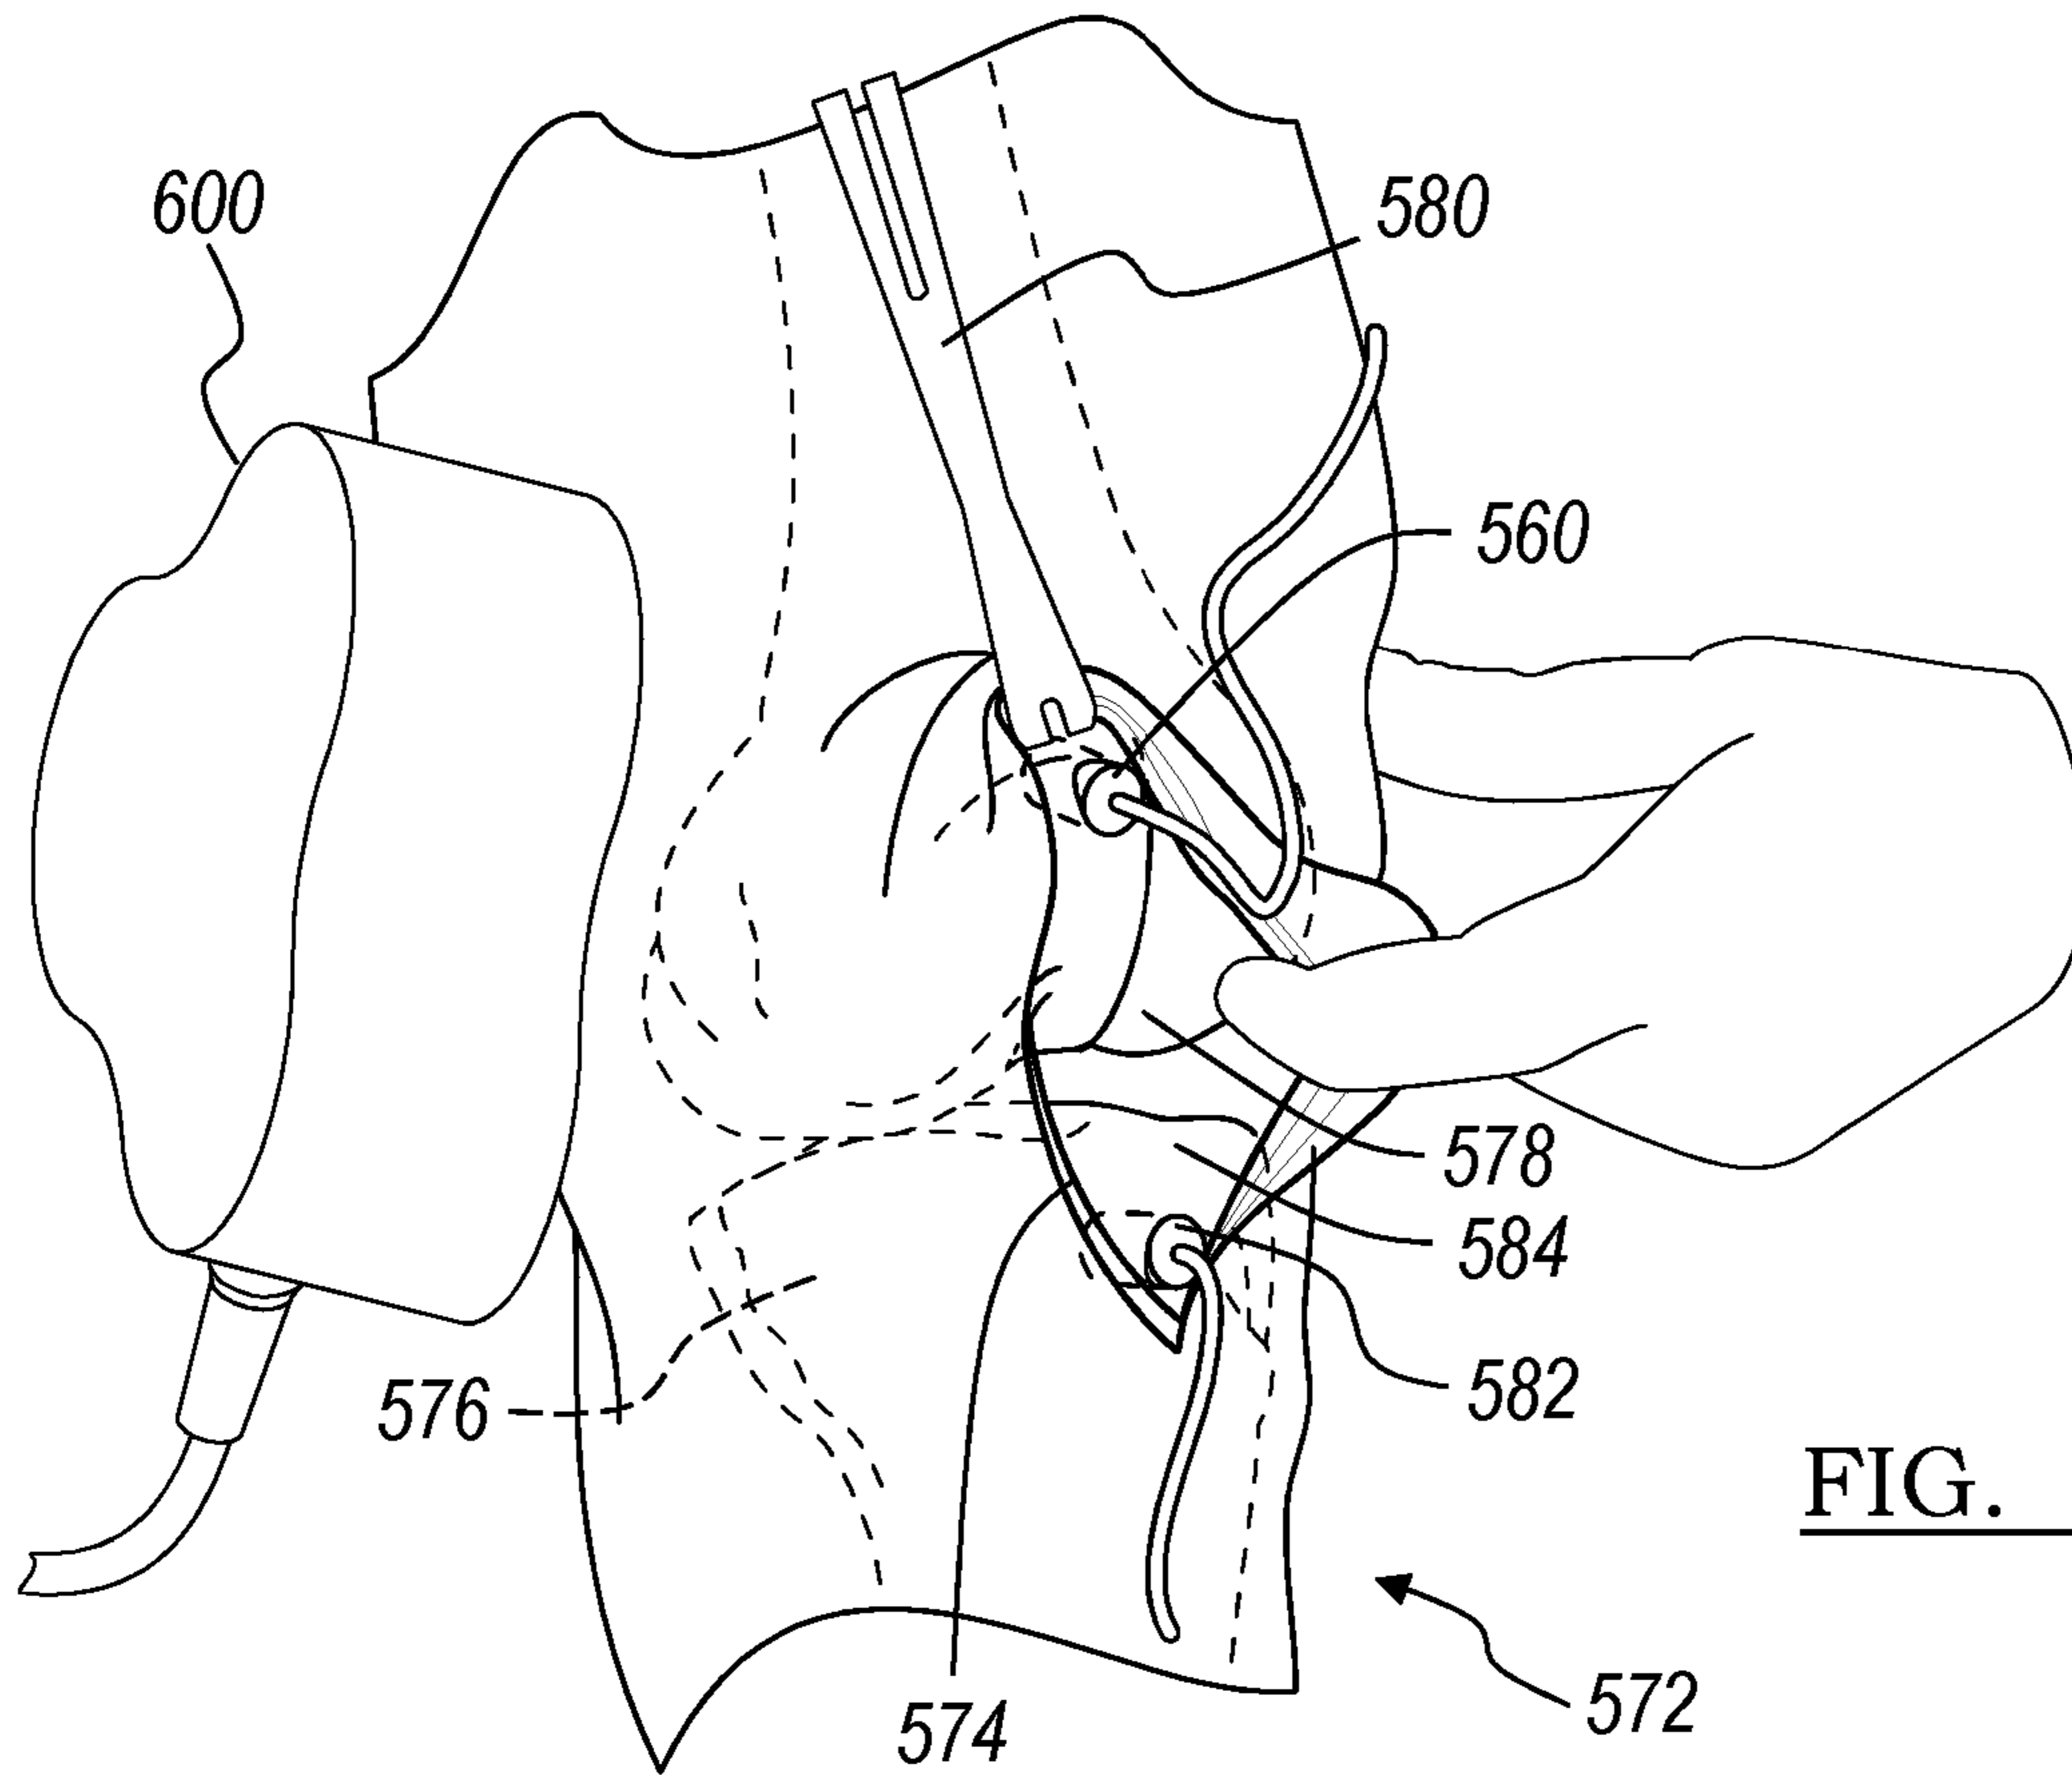


FIG. 28D

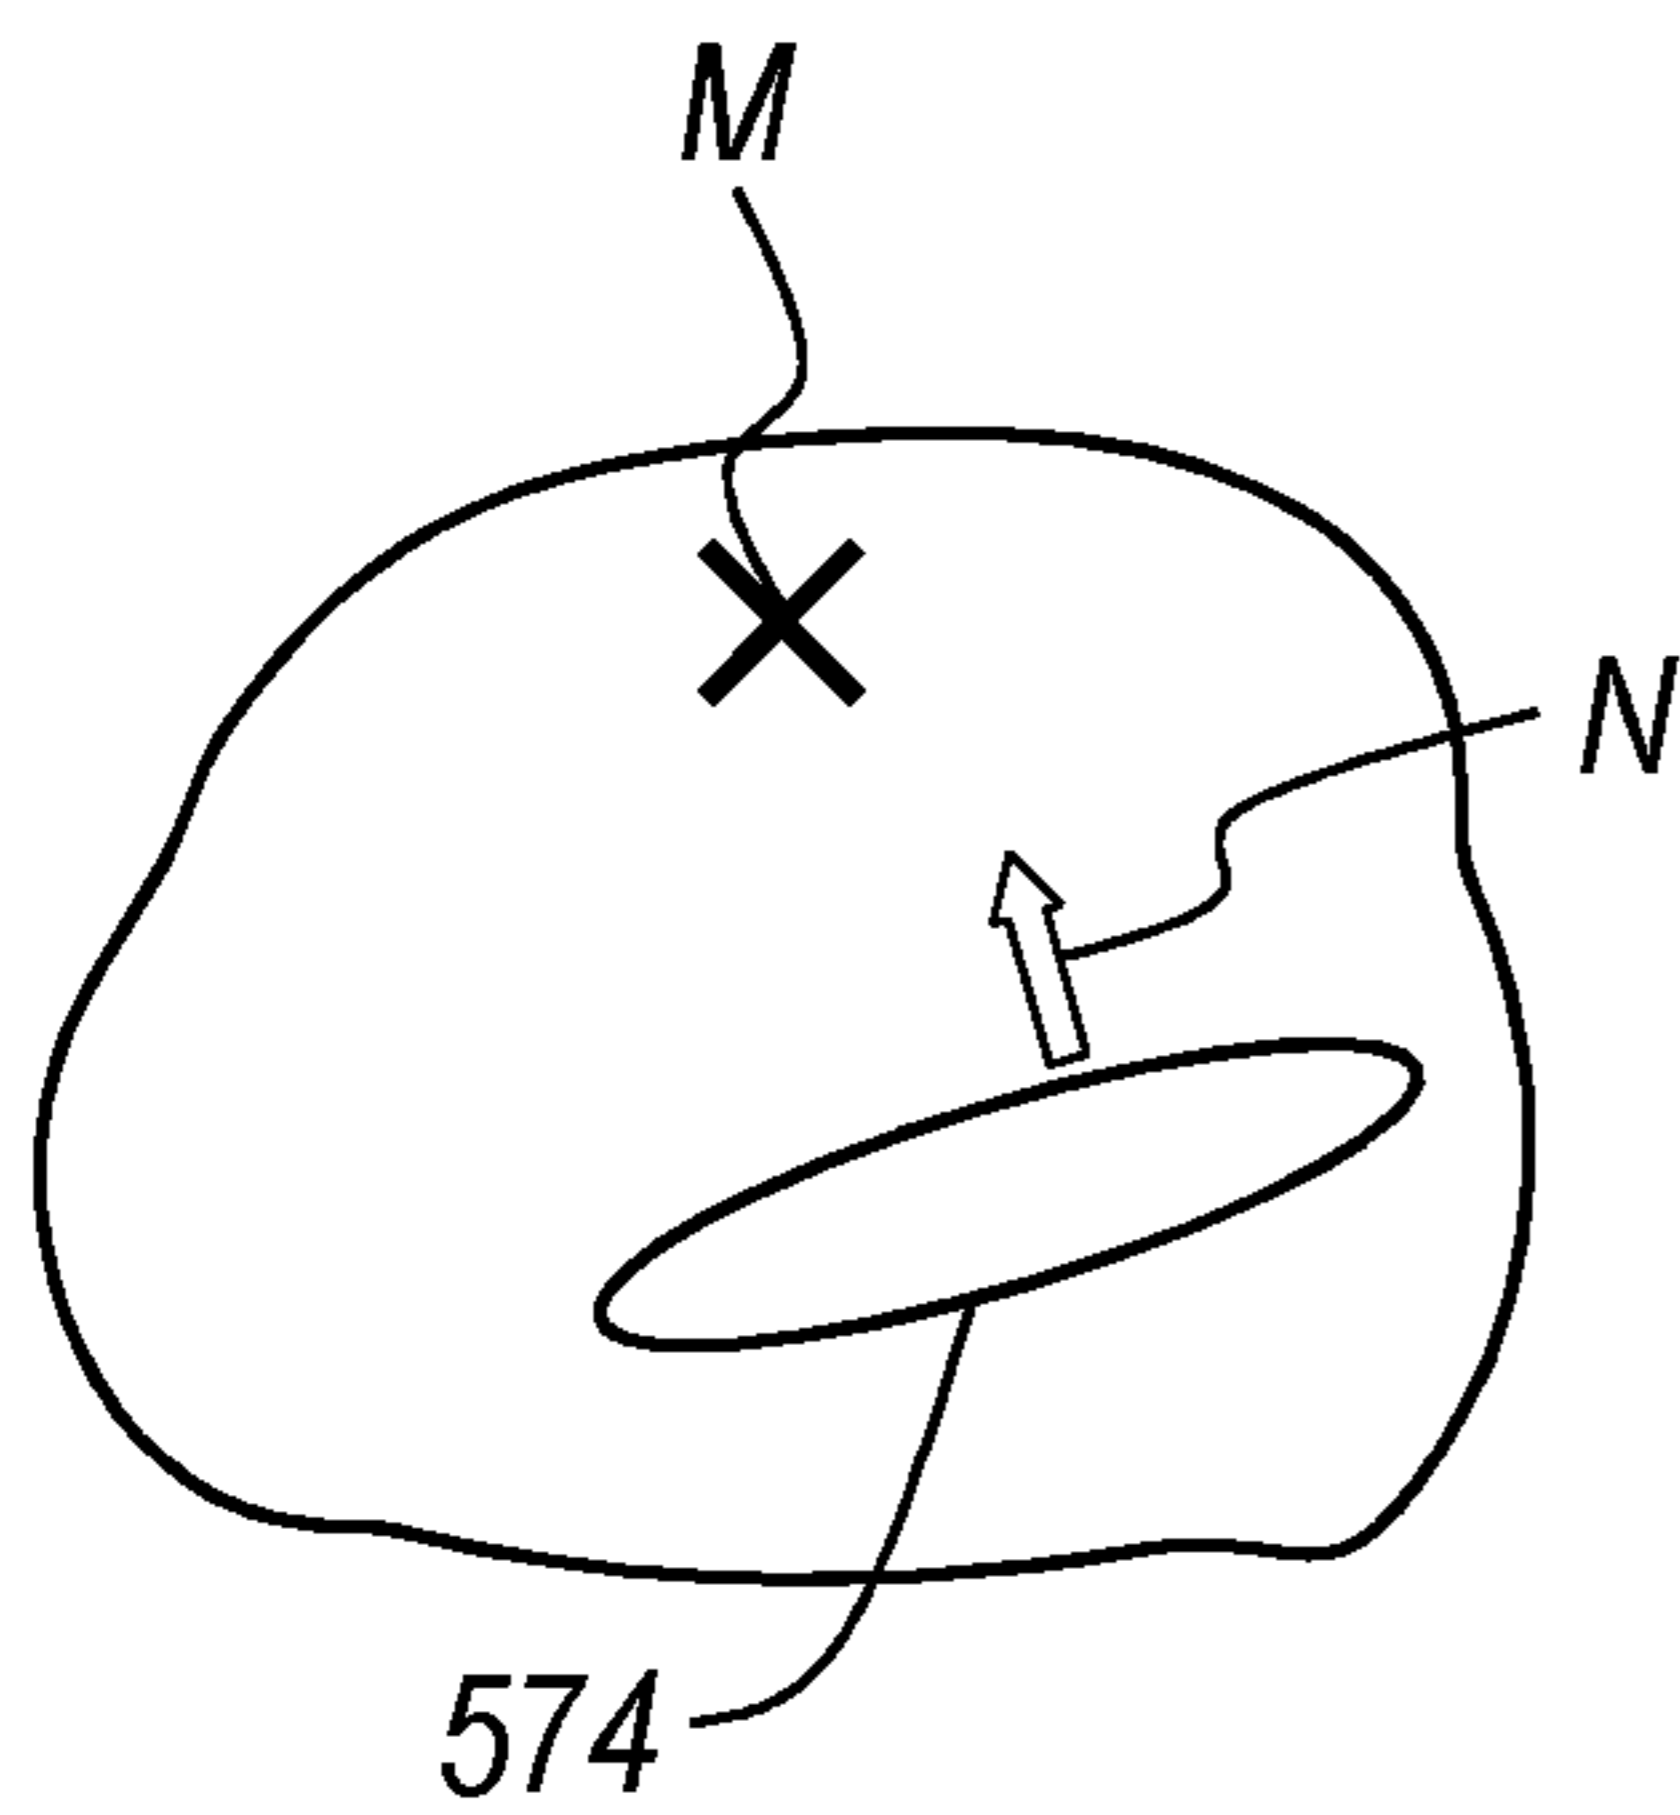


FIG. 28A

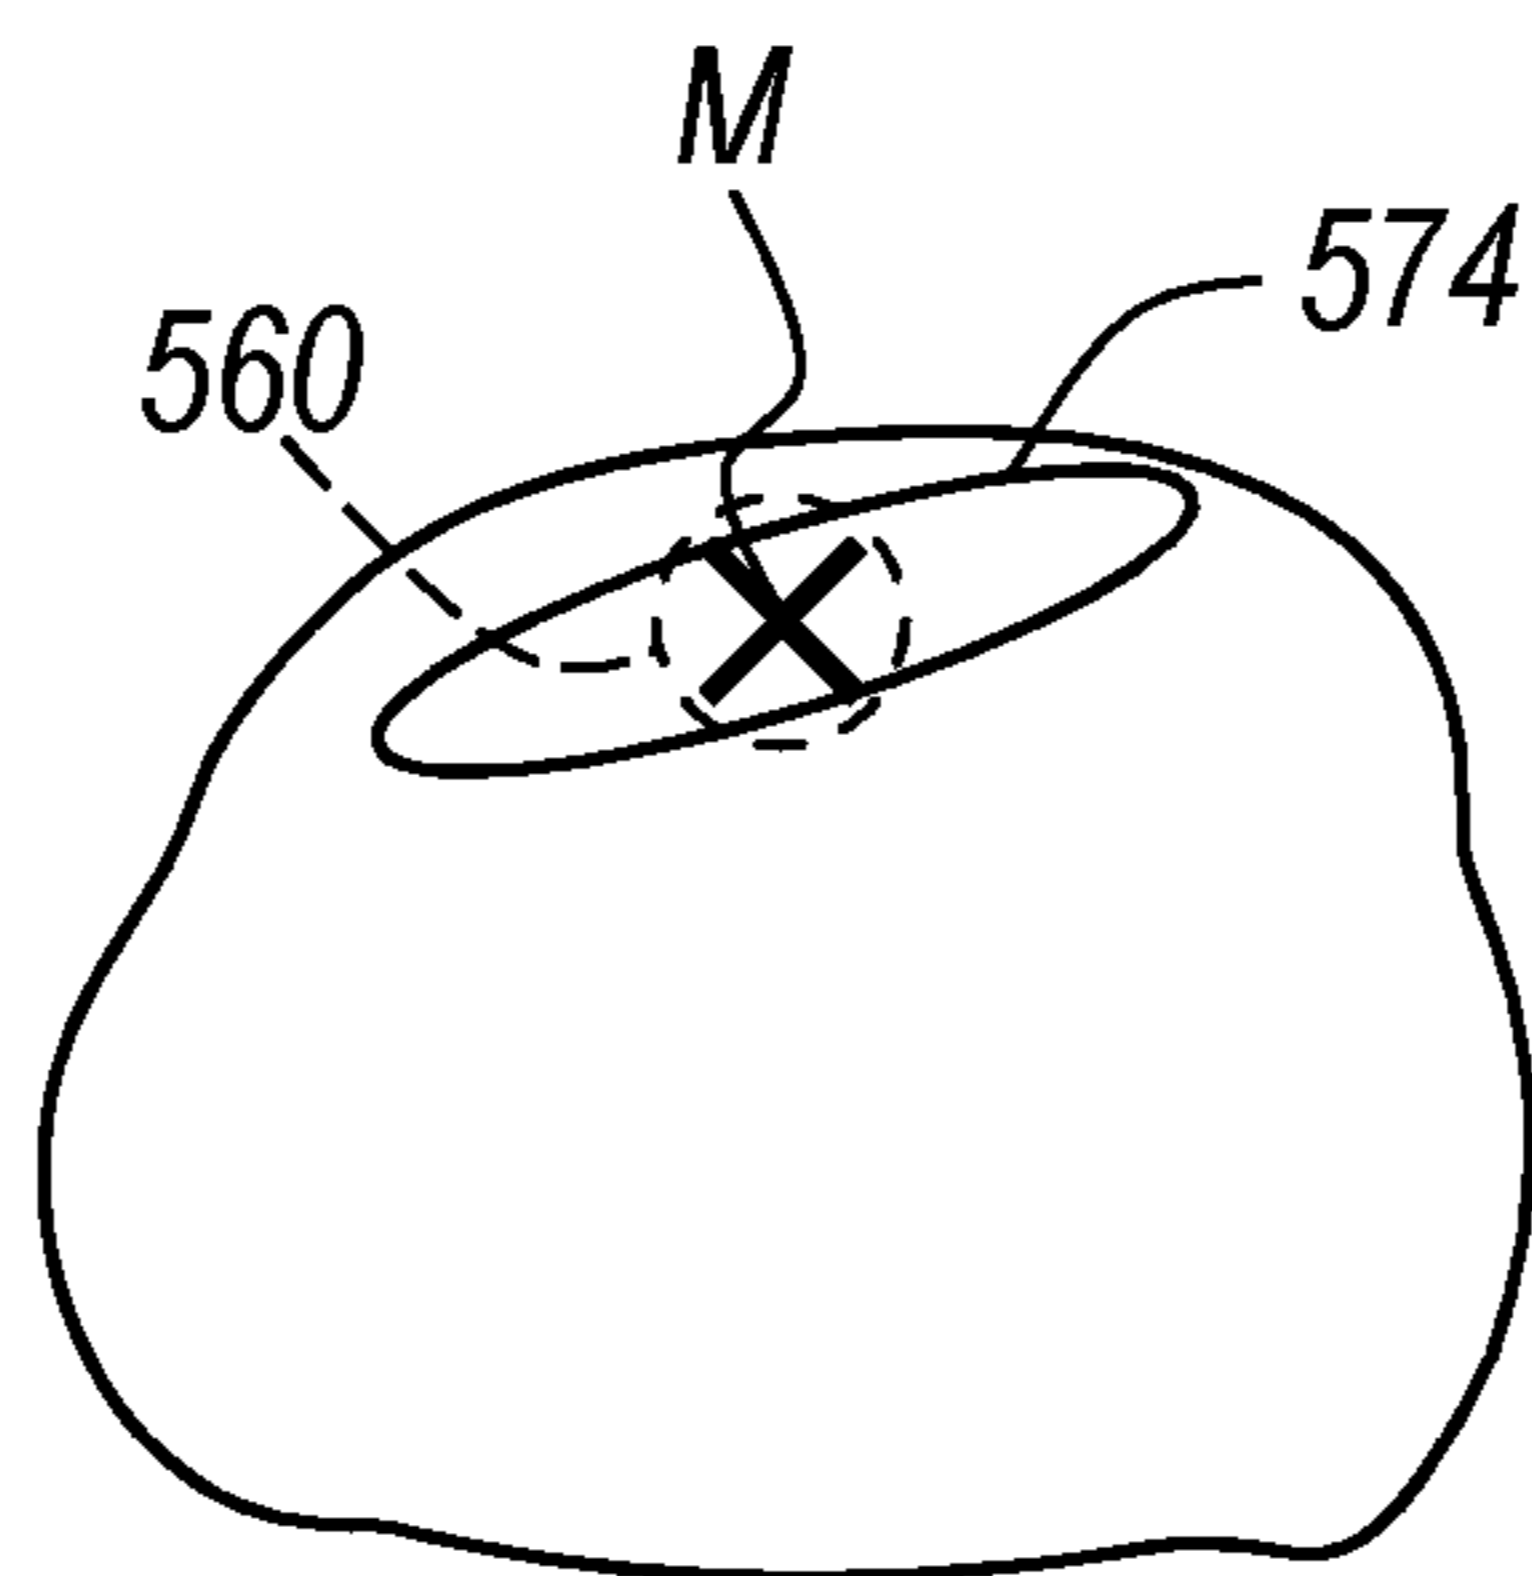


FIG. 28B

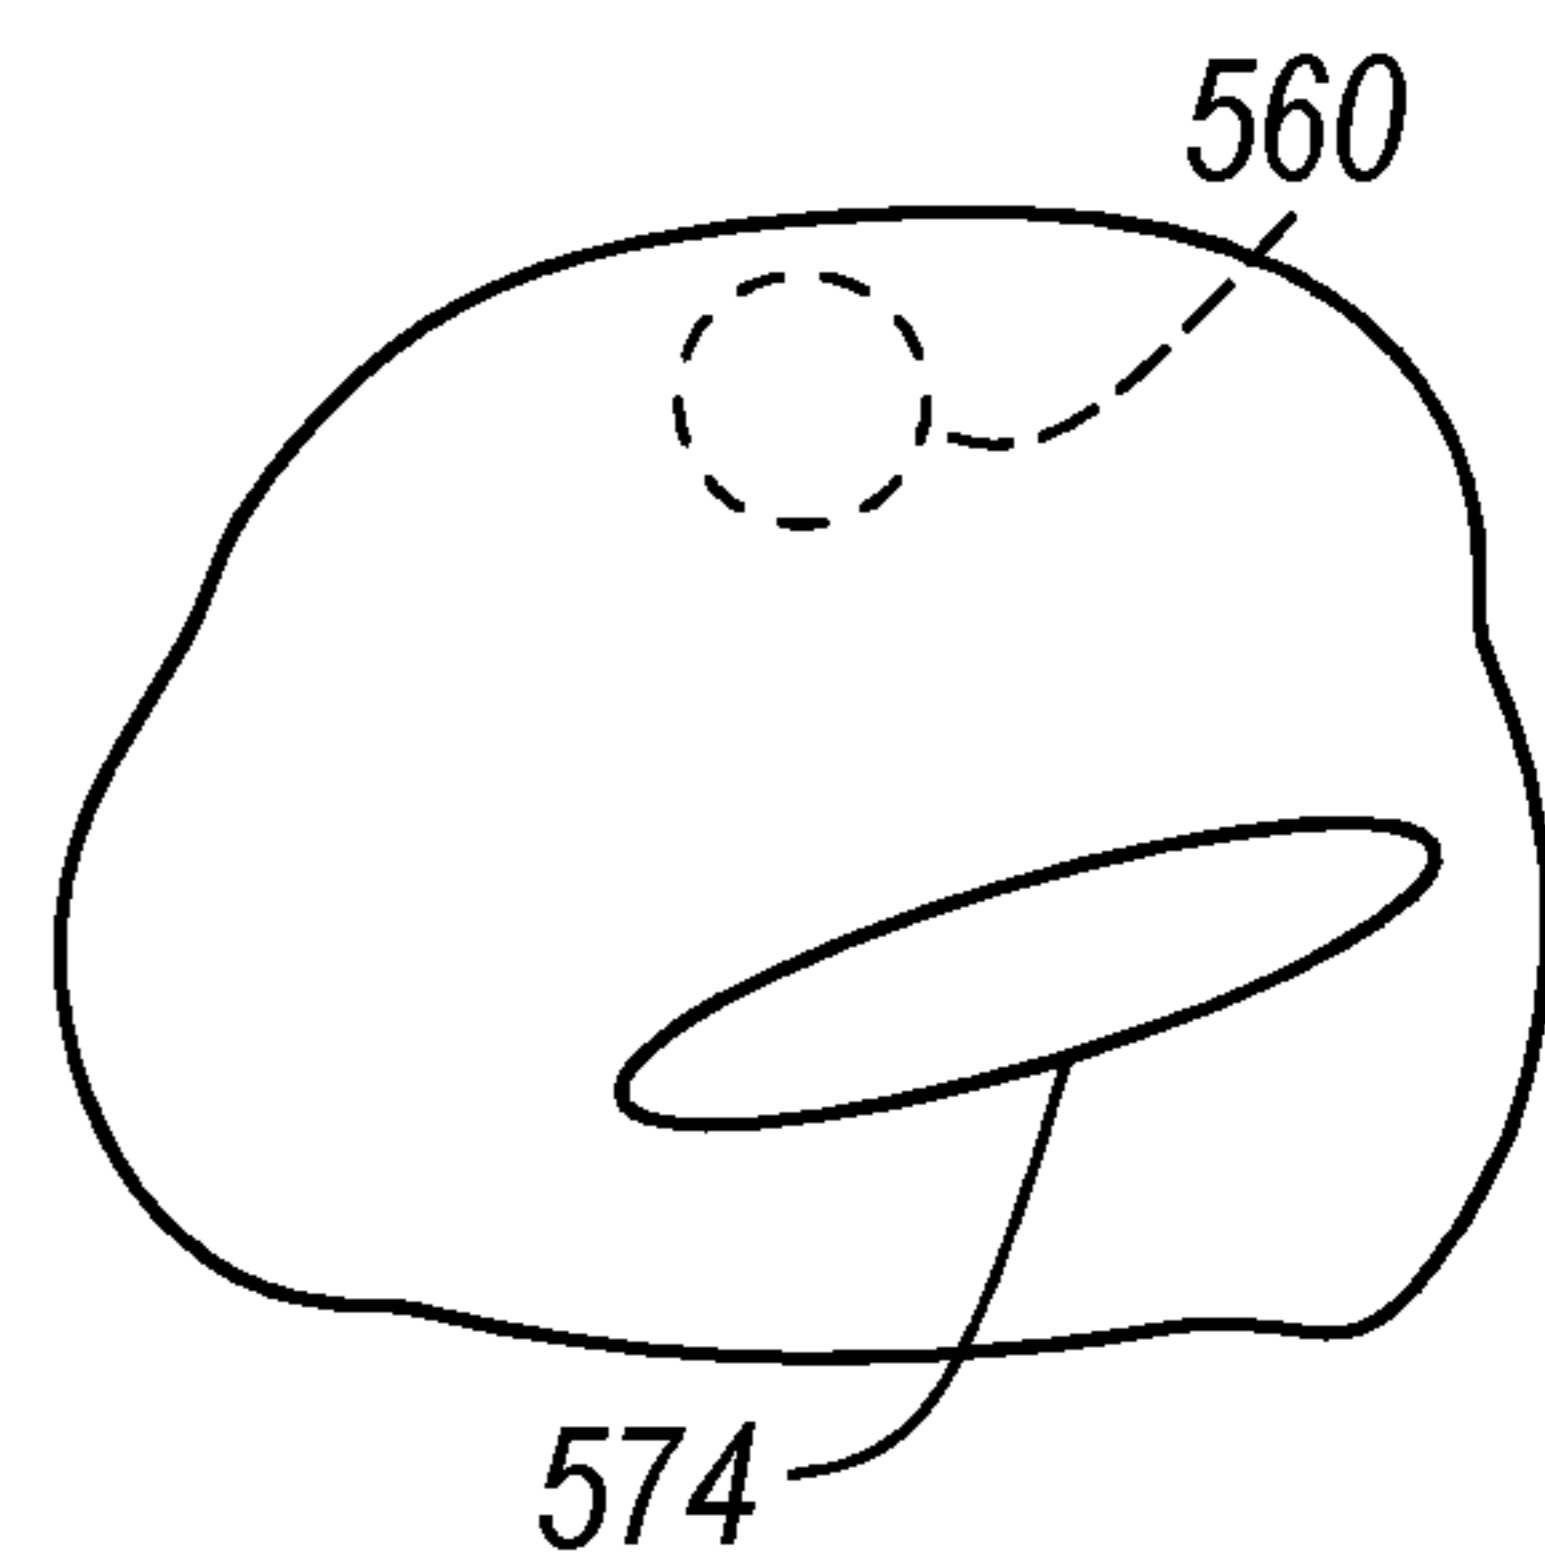


FIG. 28C

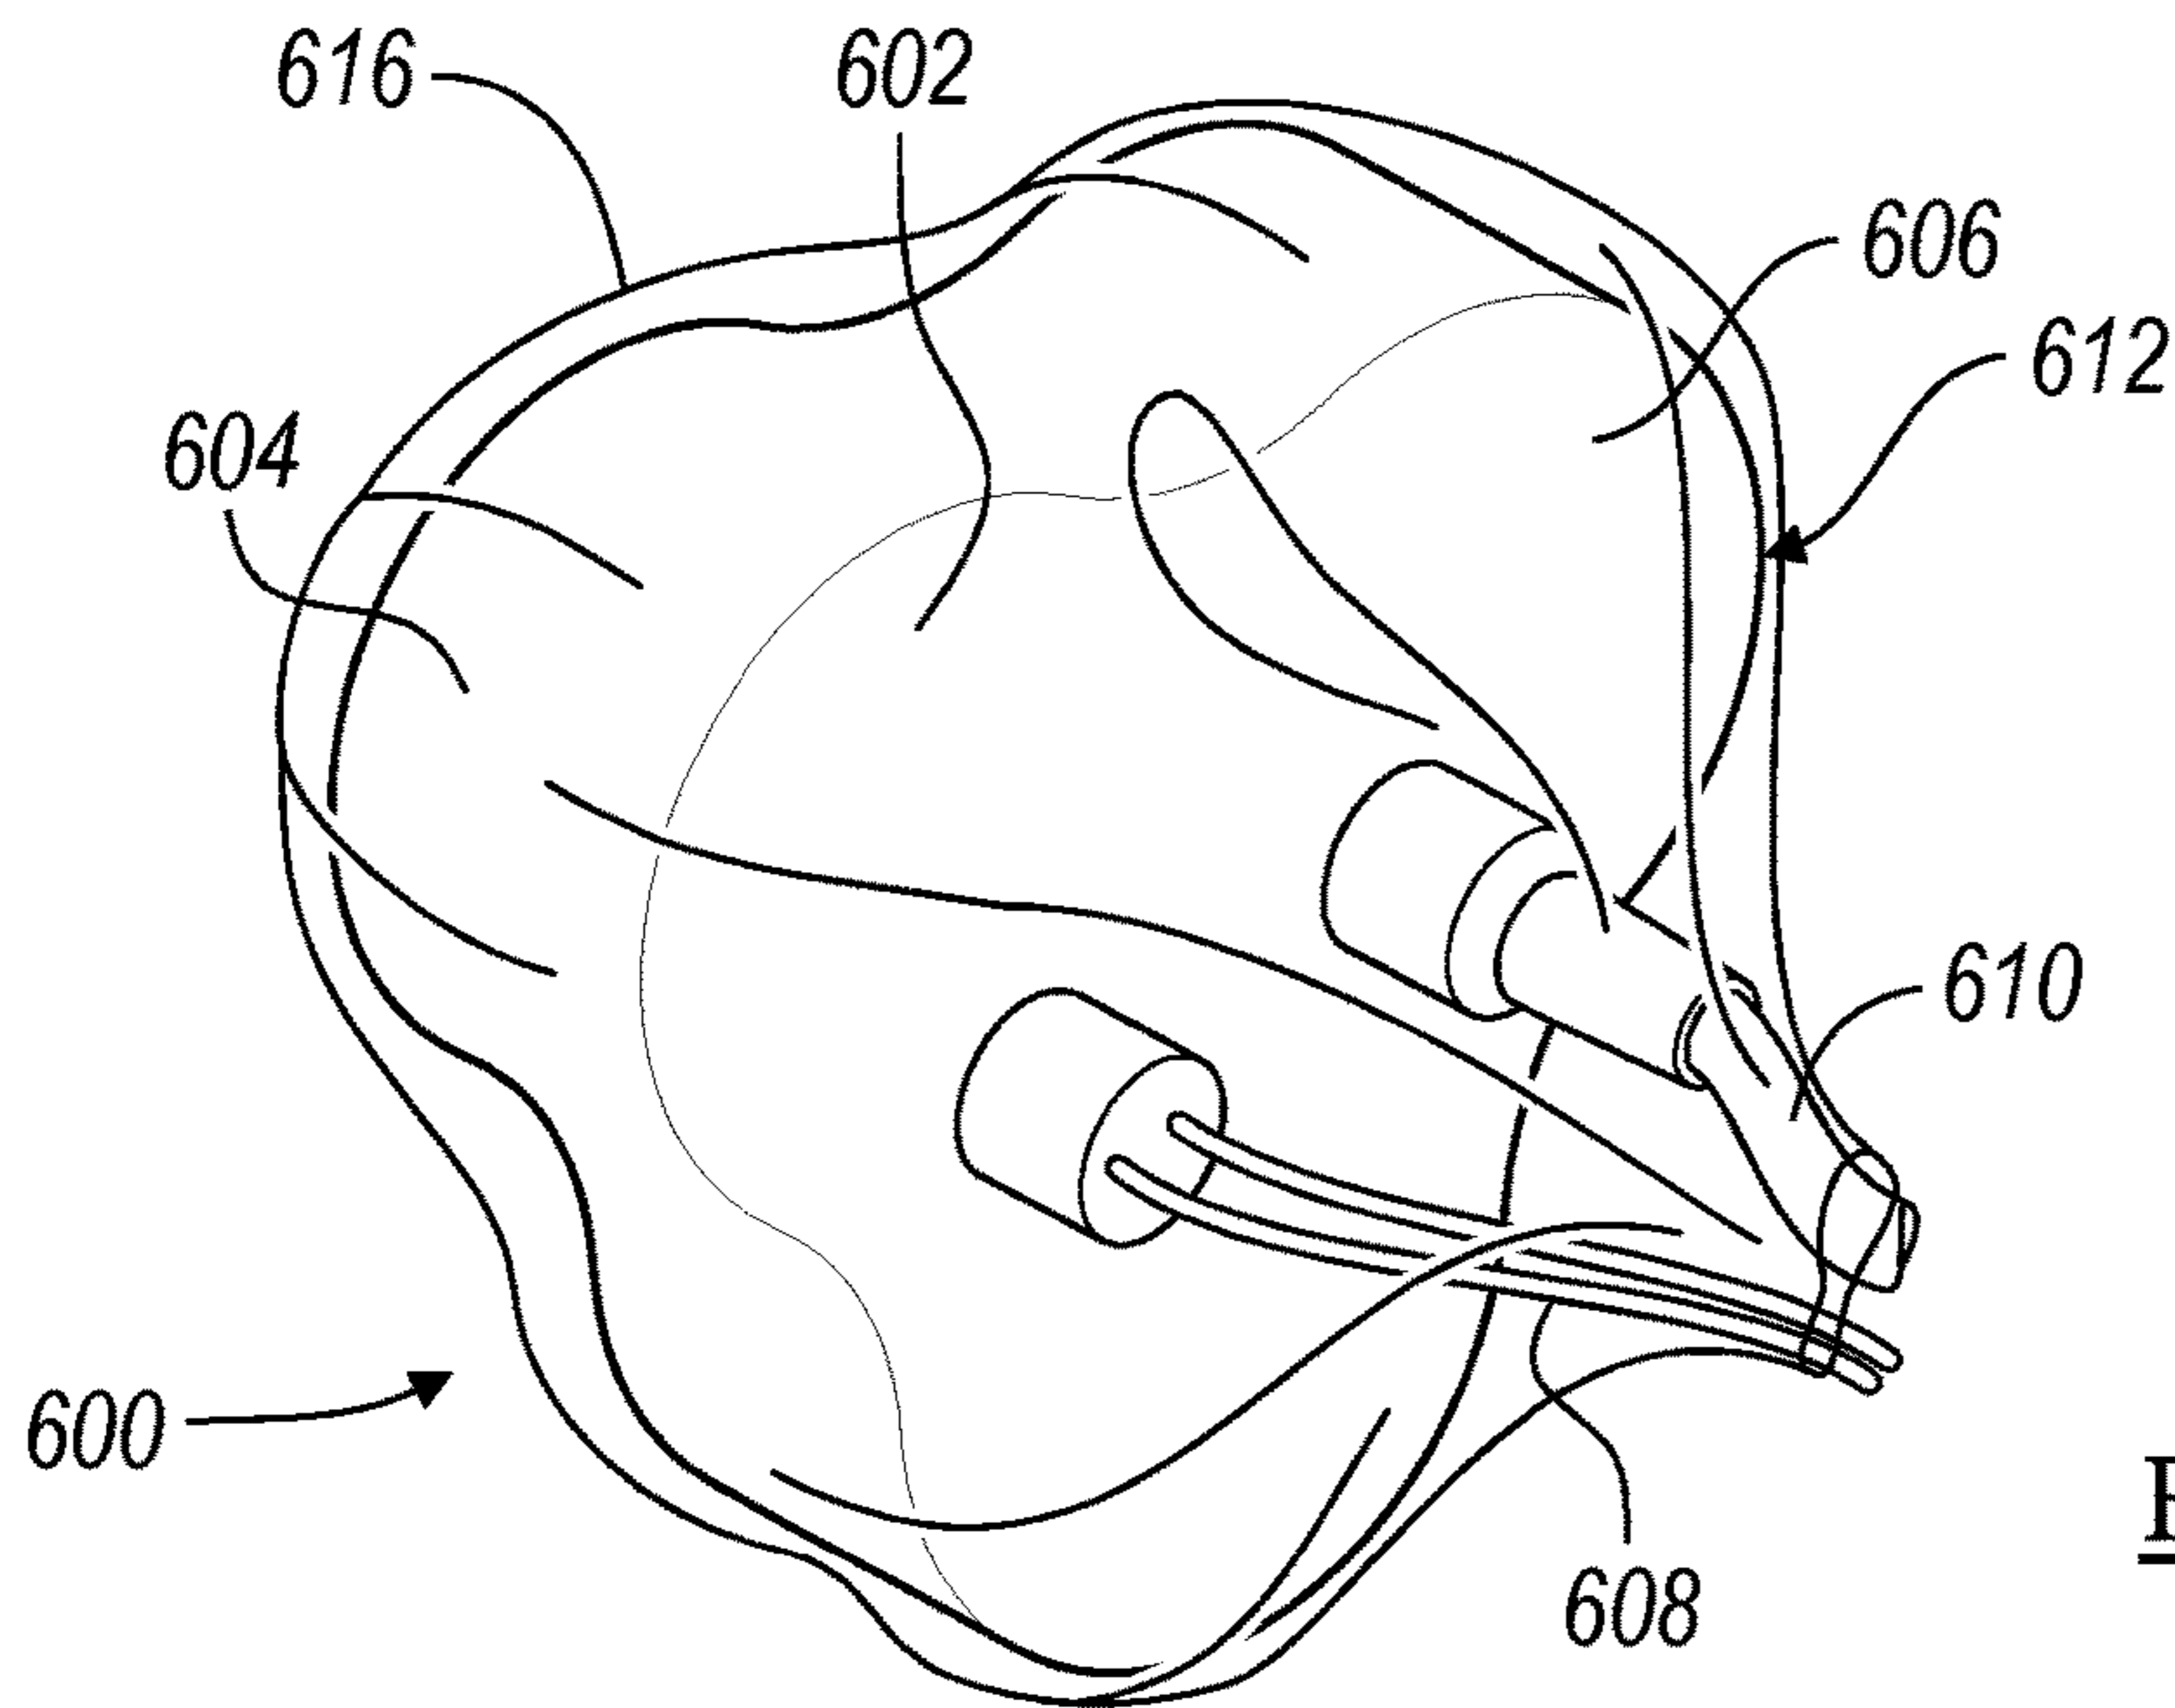


FIG. 29

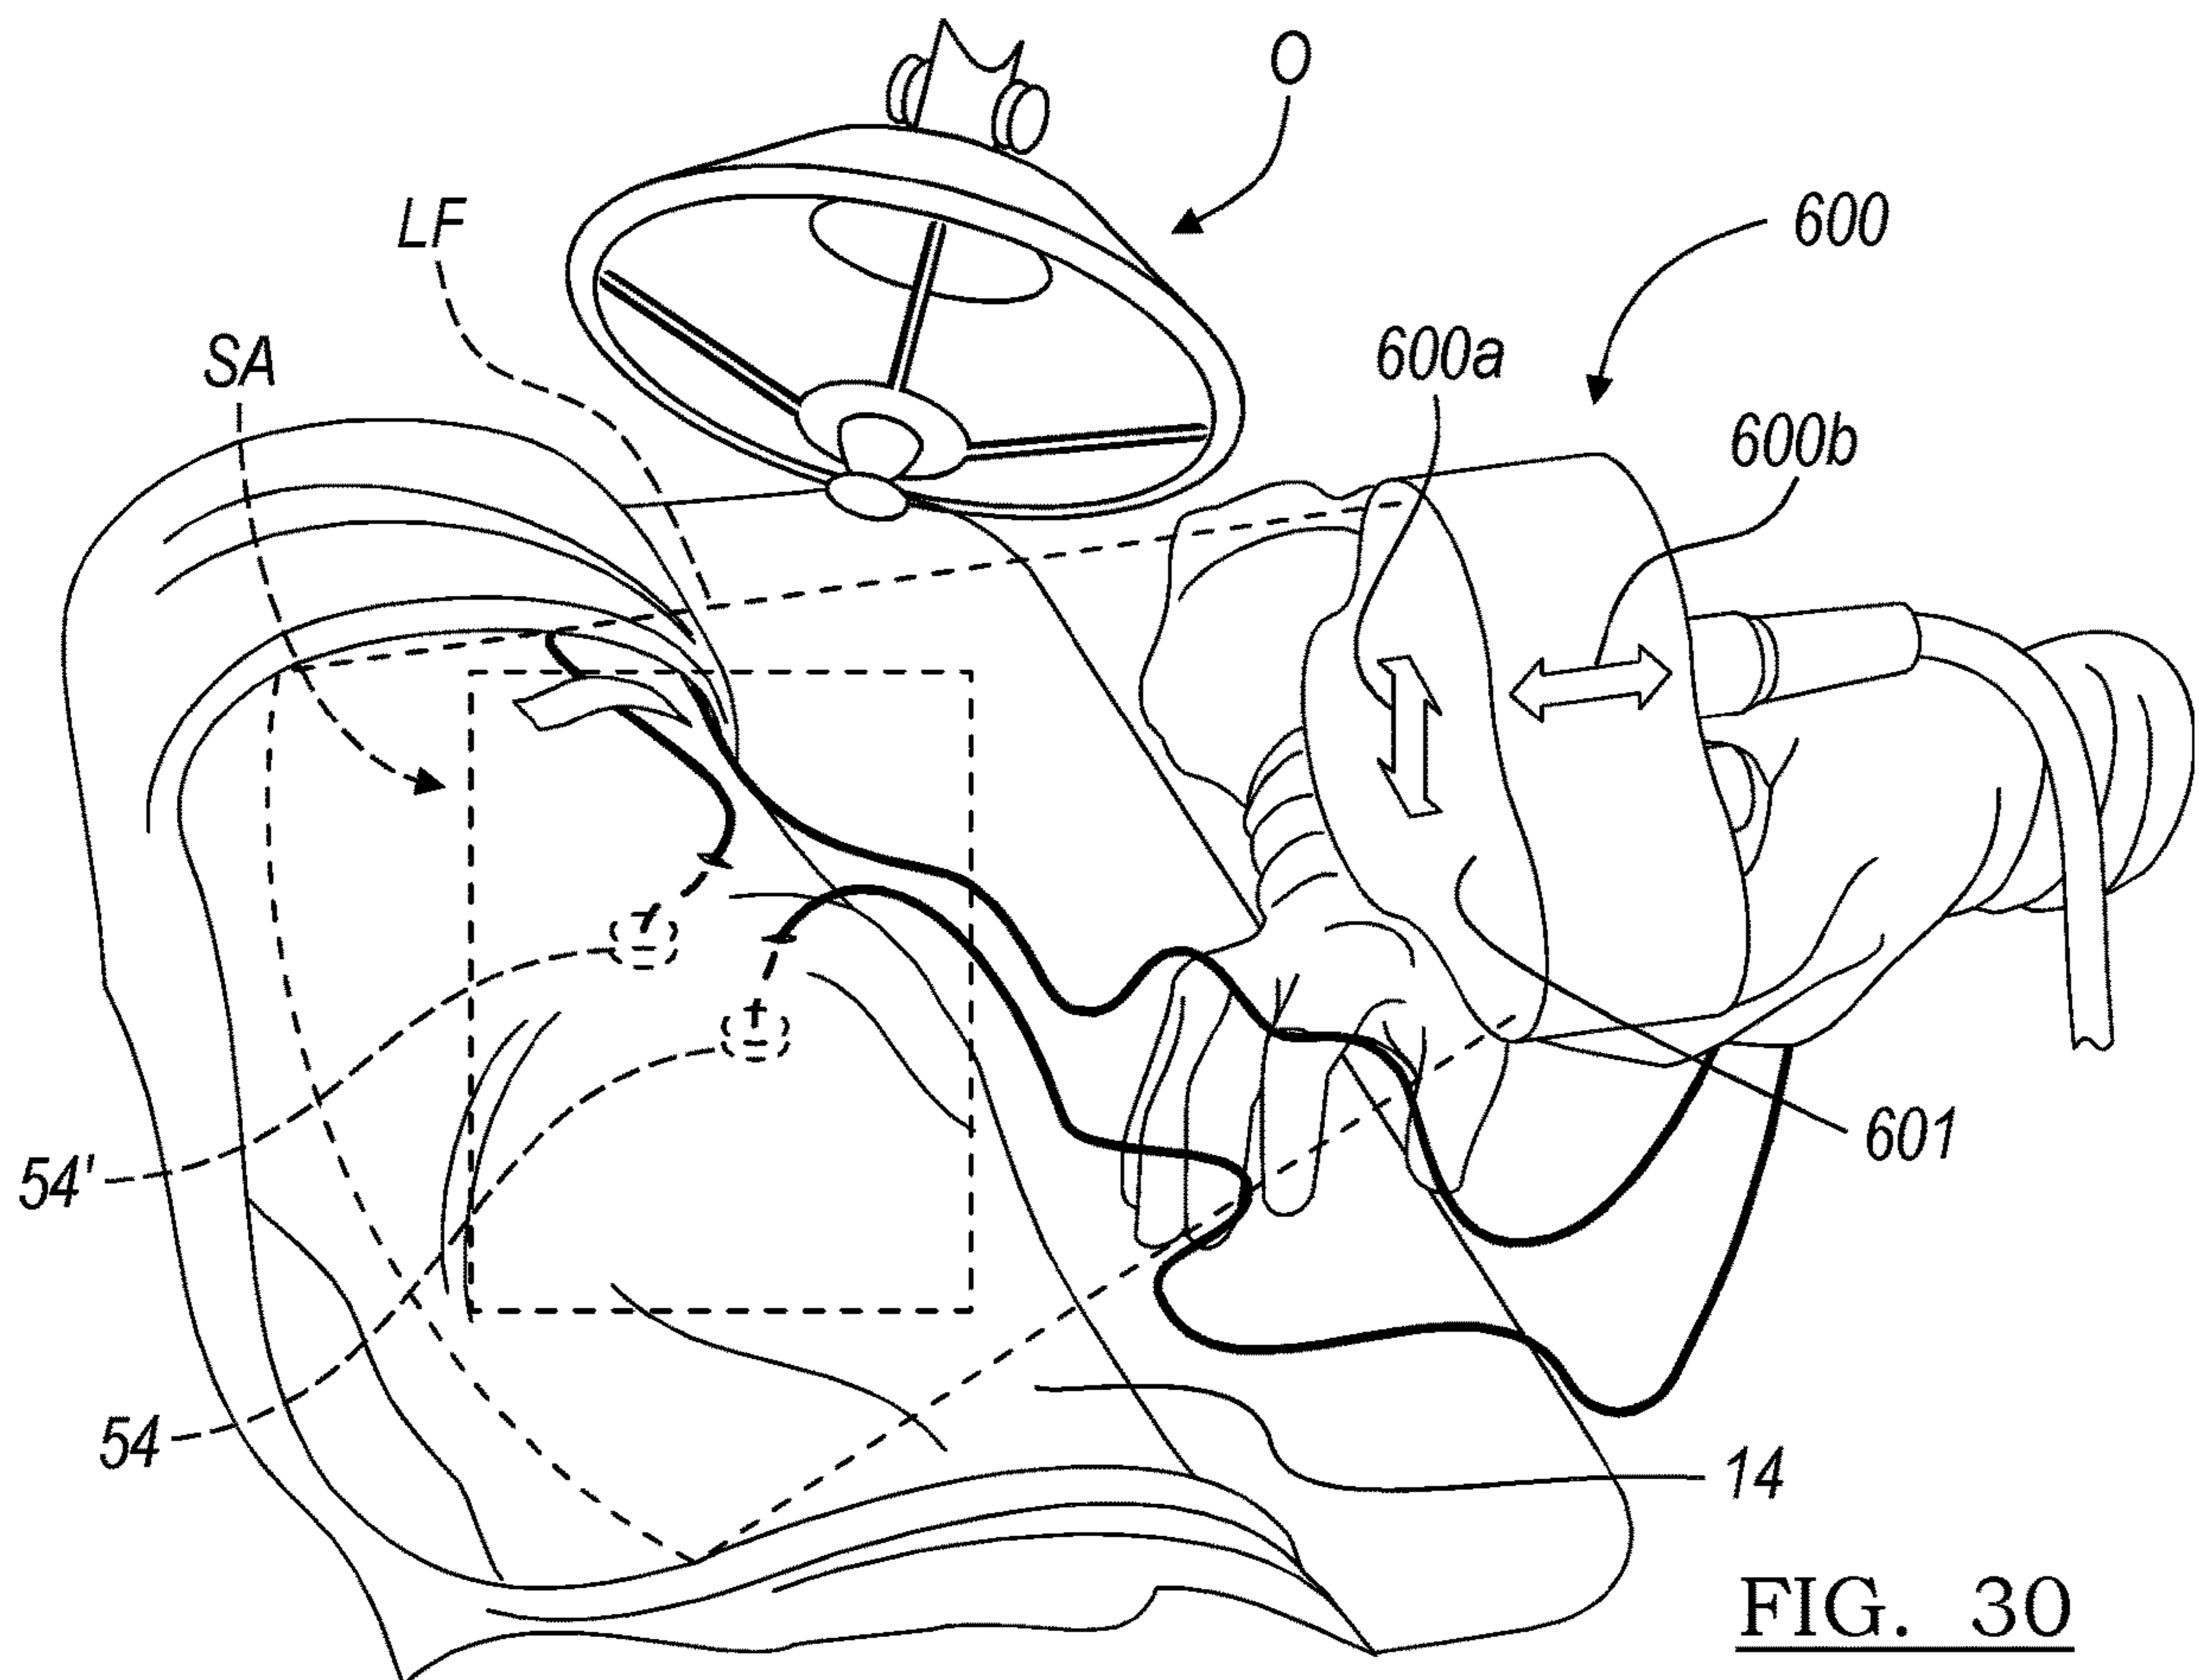


FIG. 30

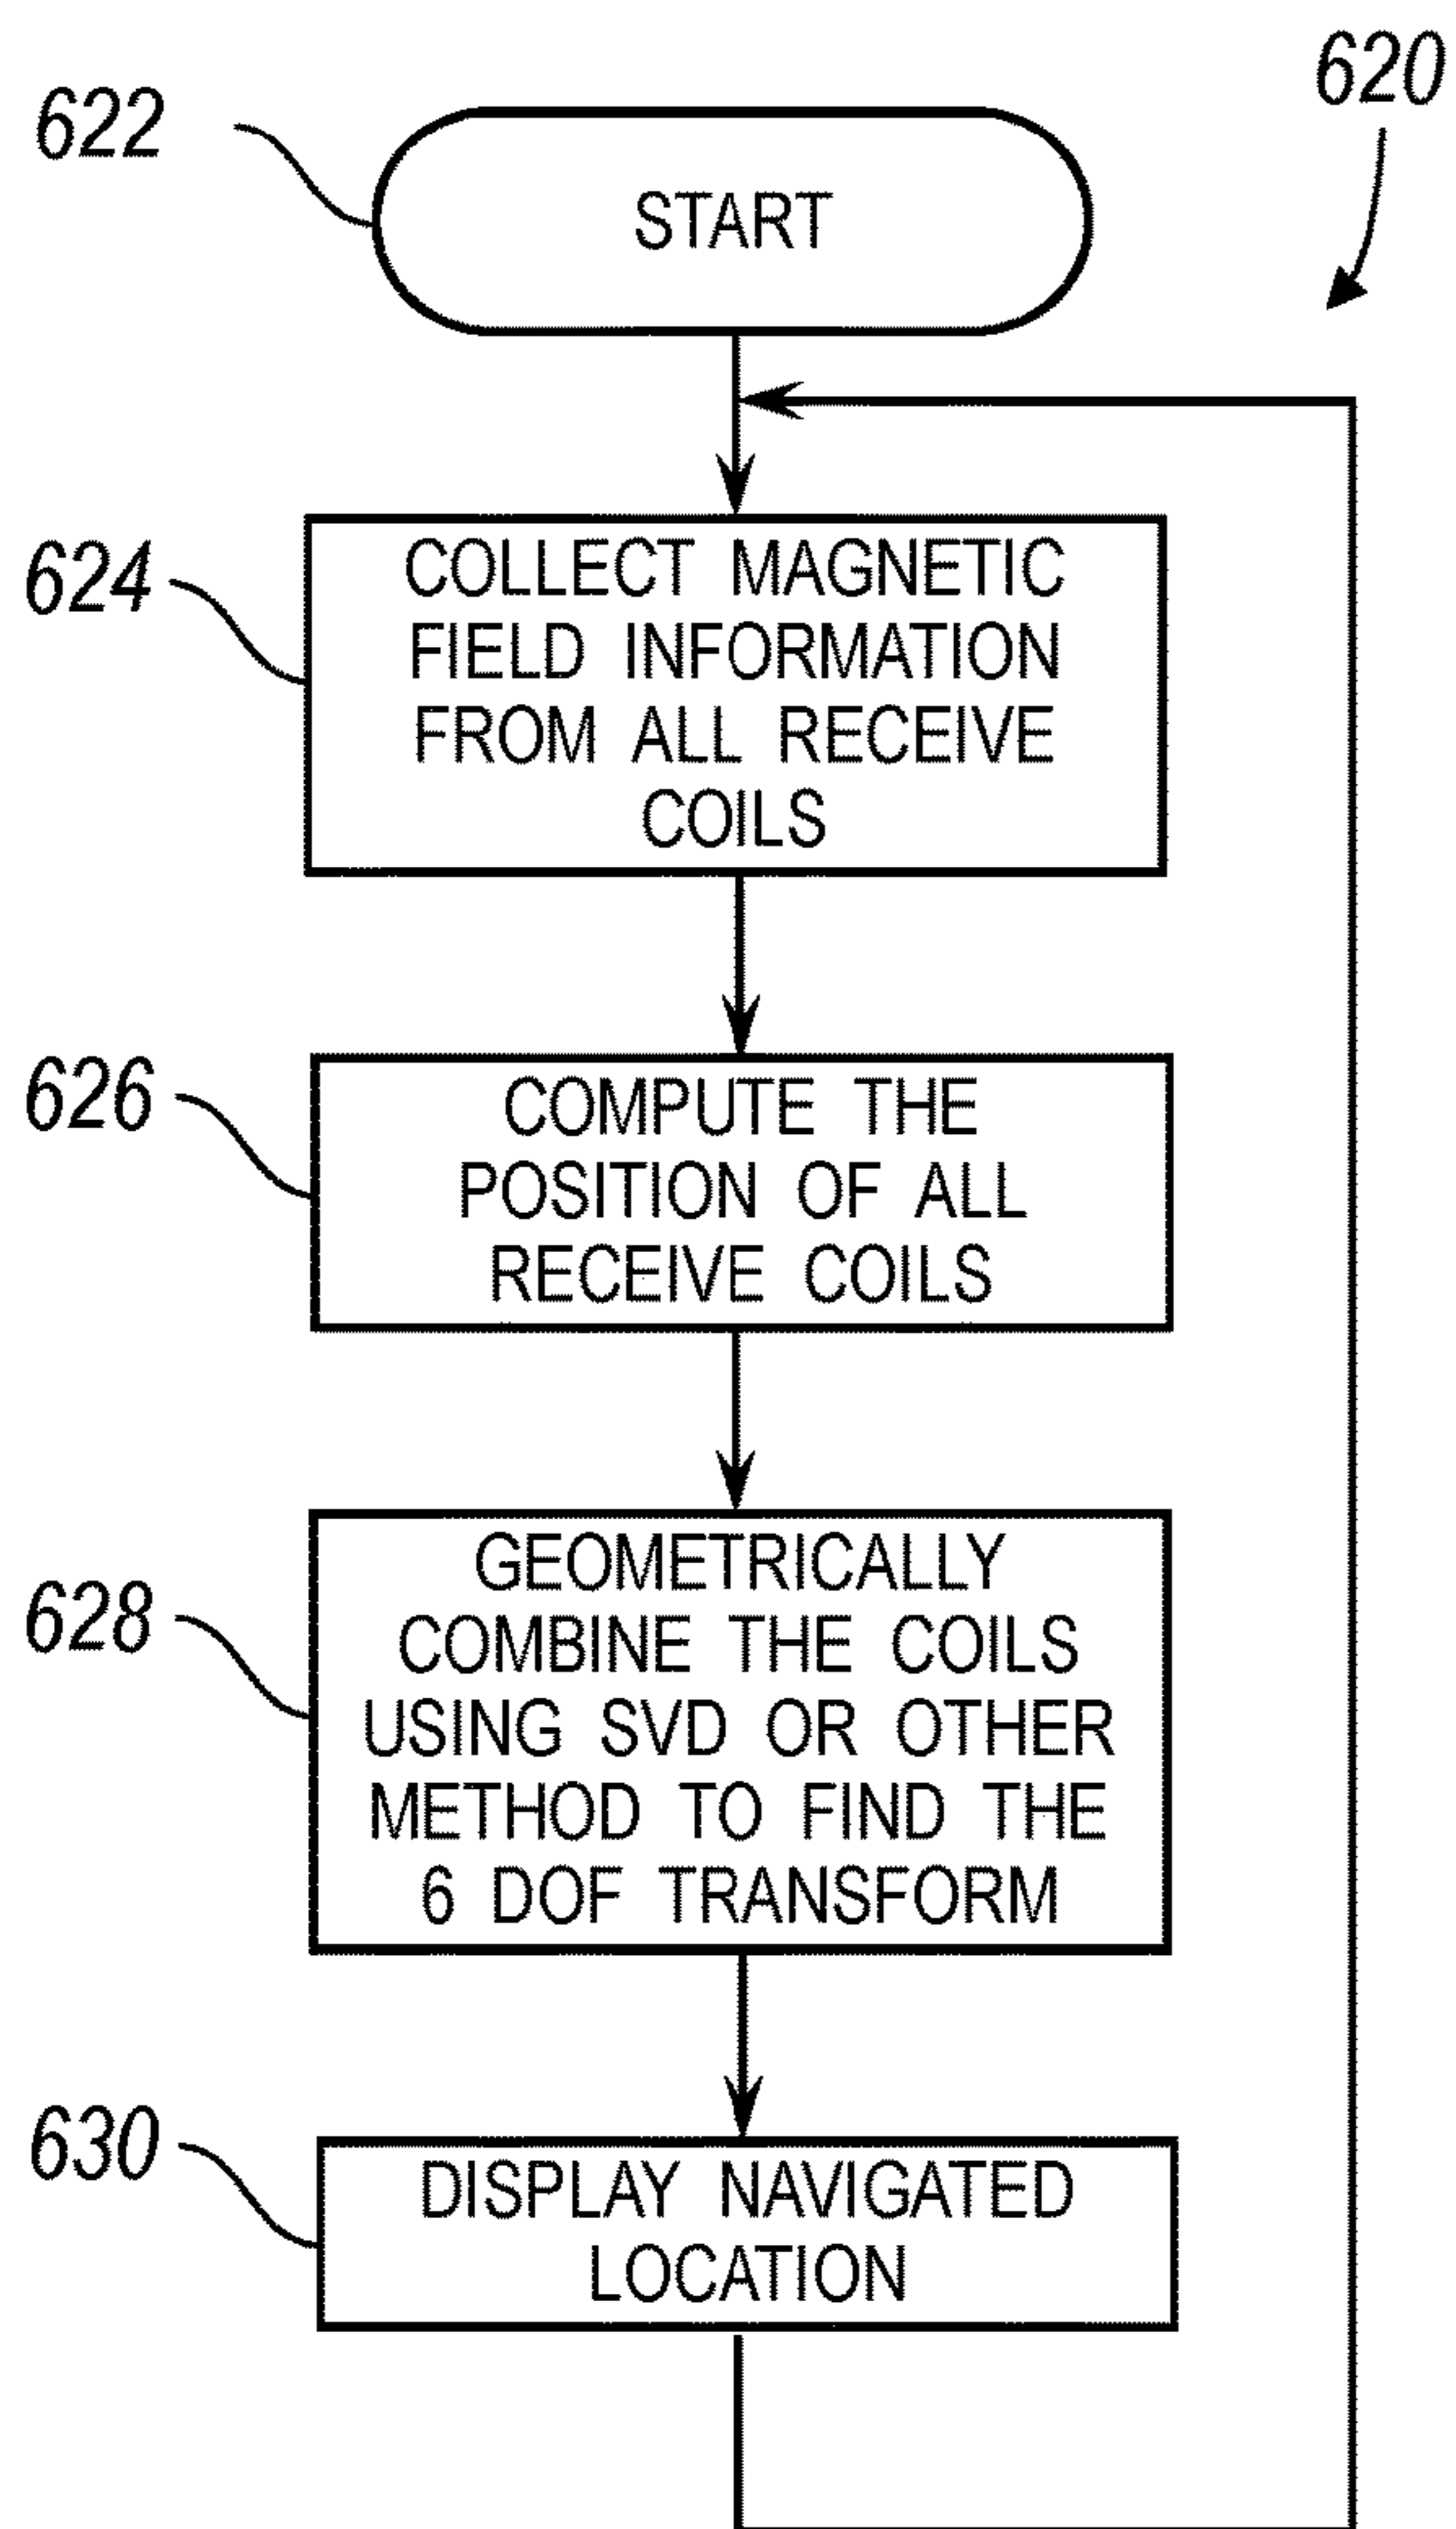


FIG. 31

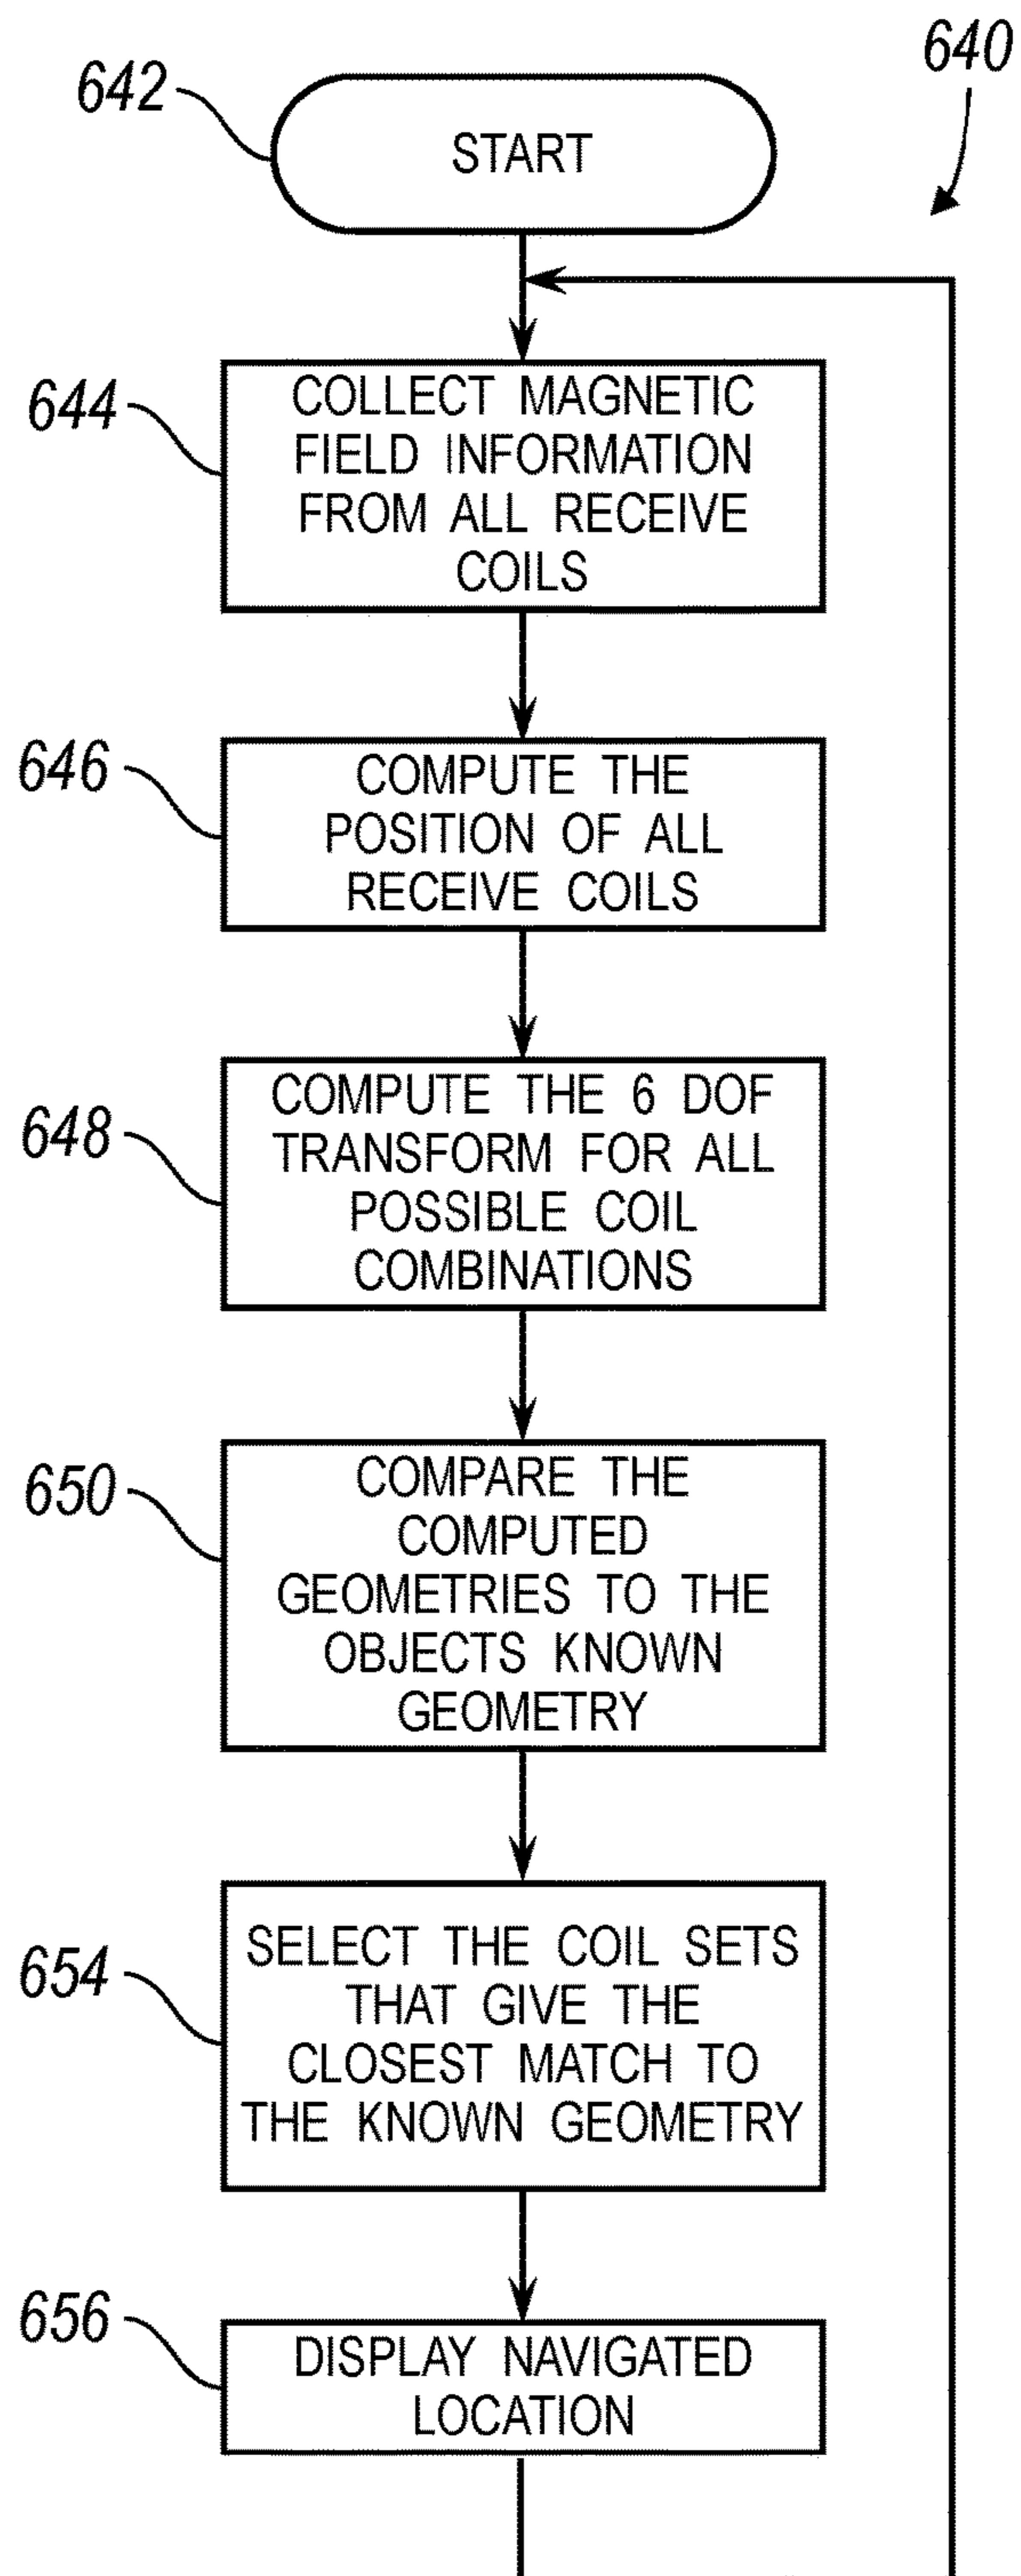
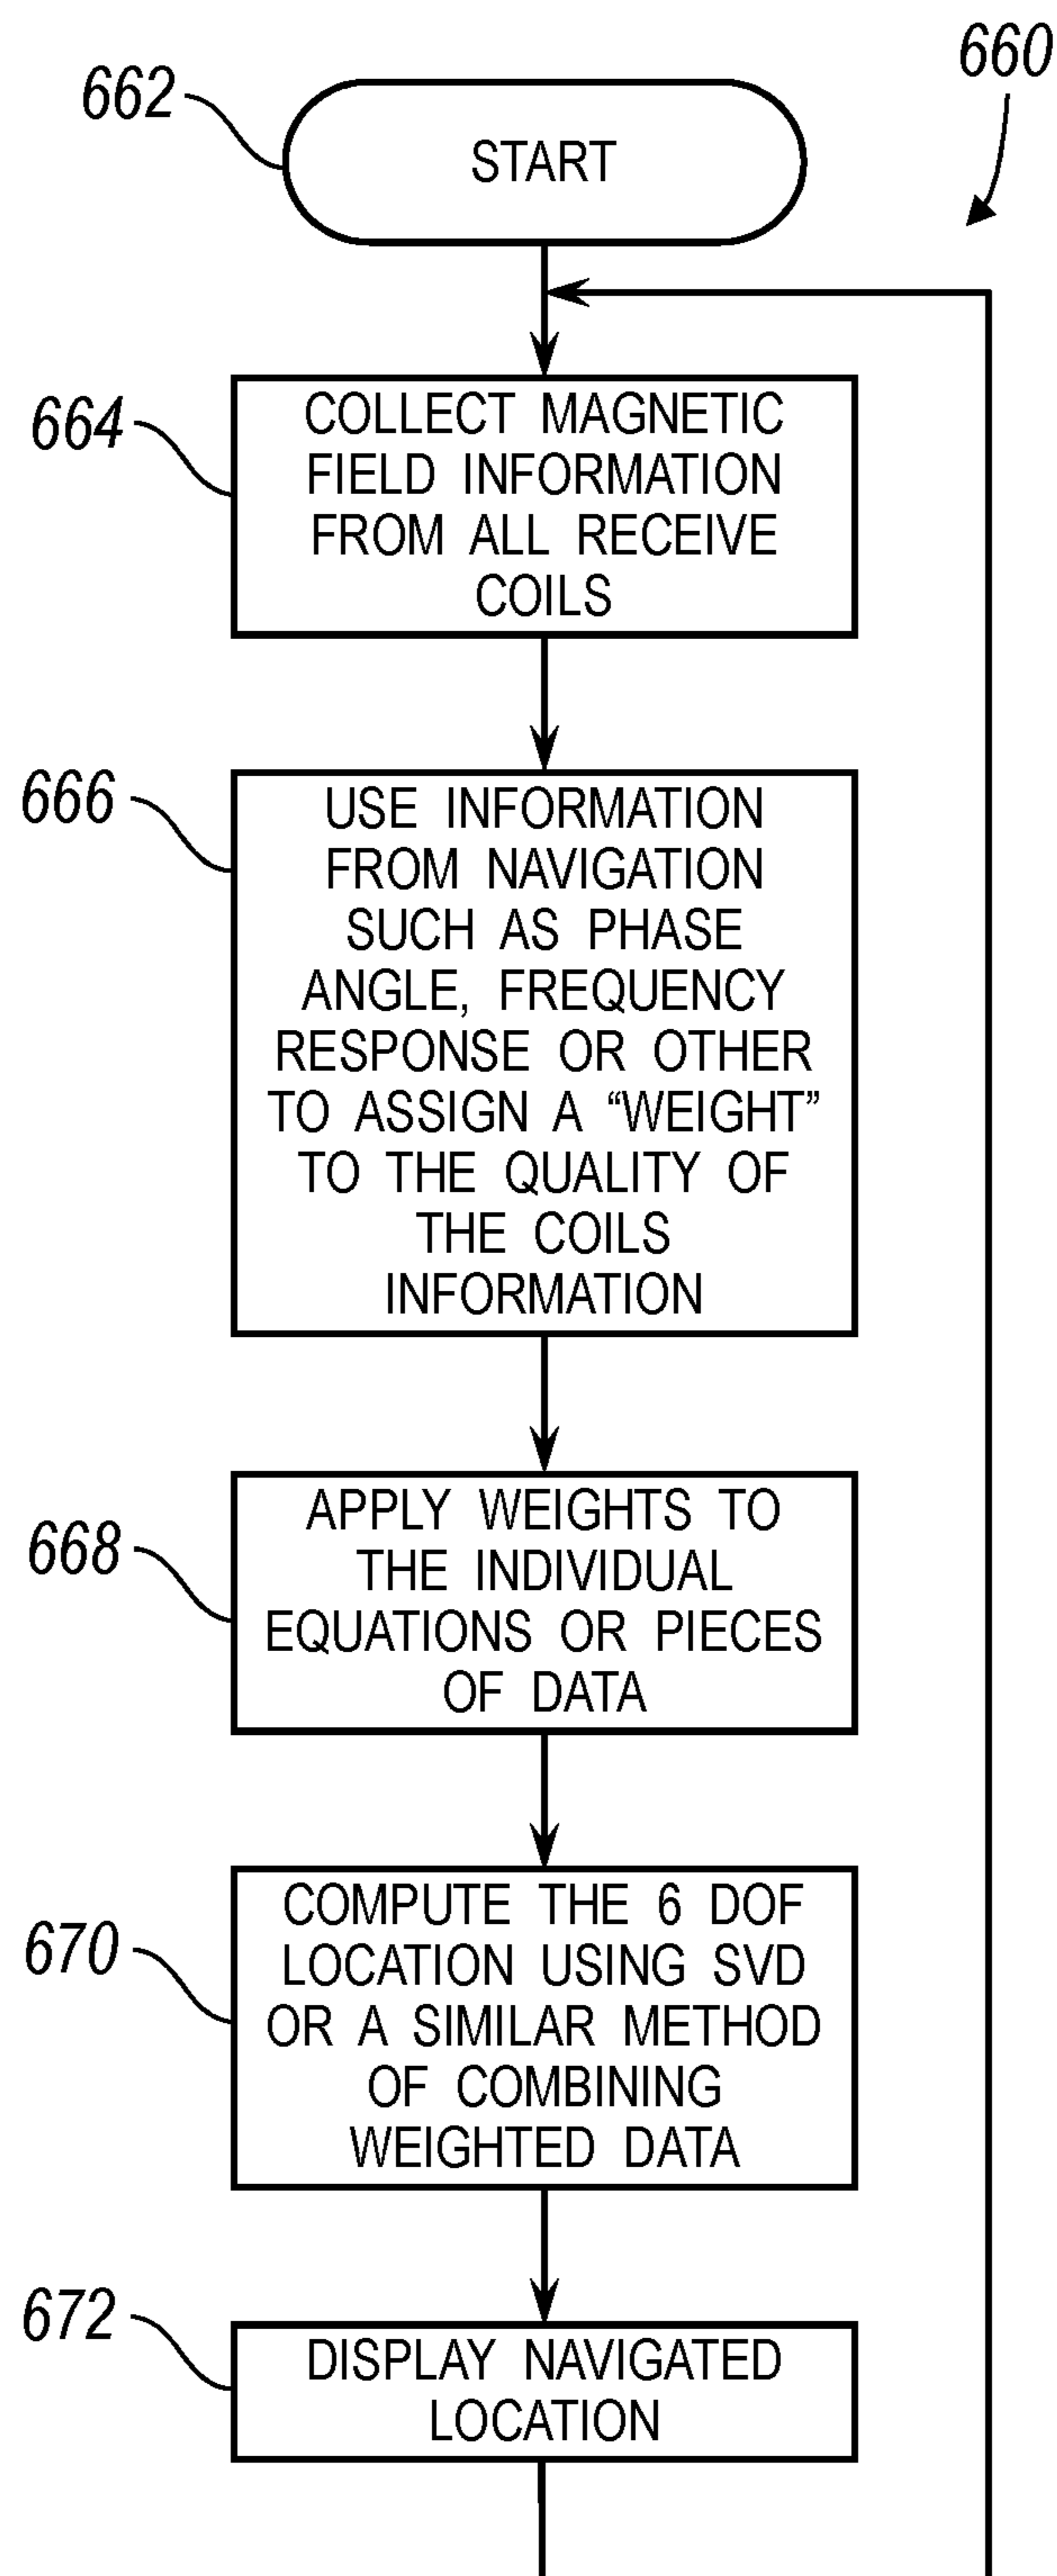


FIG. 32

FIG. 33

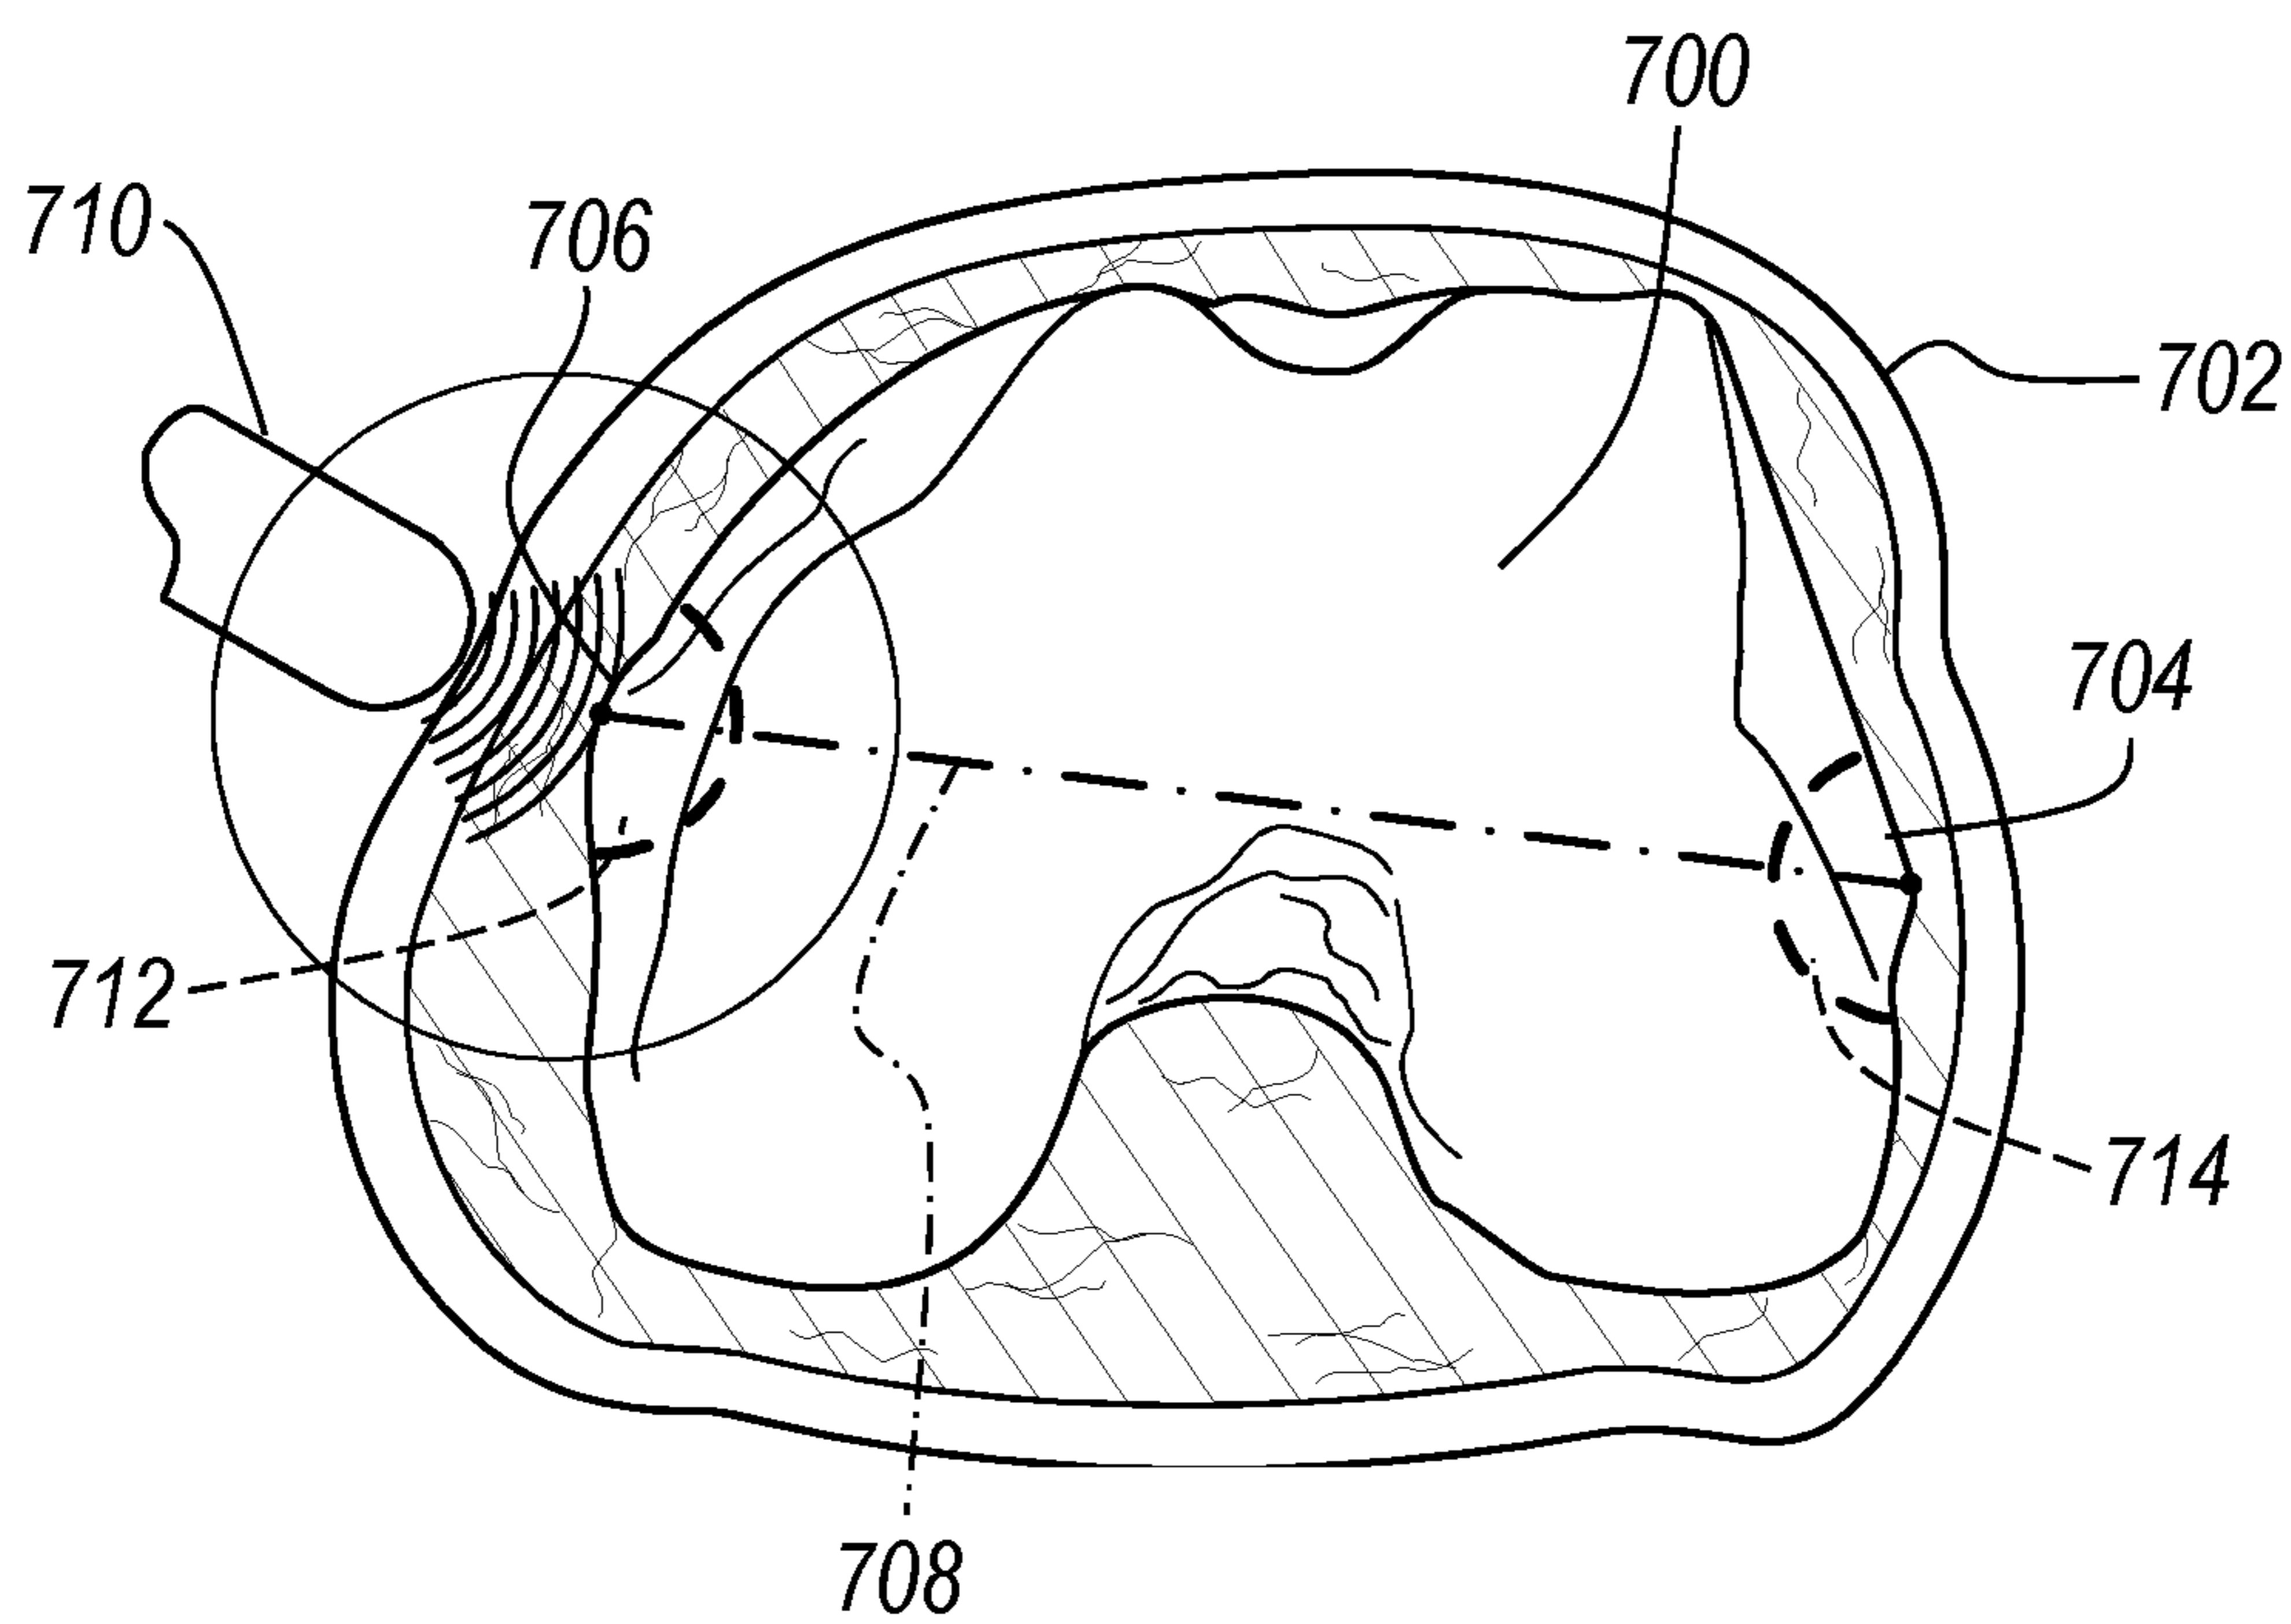


FIG. 34A

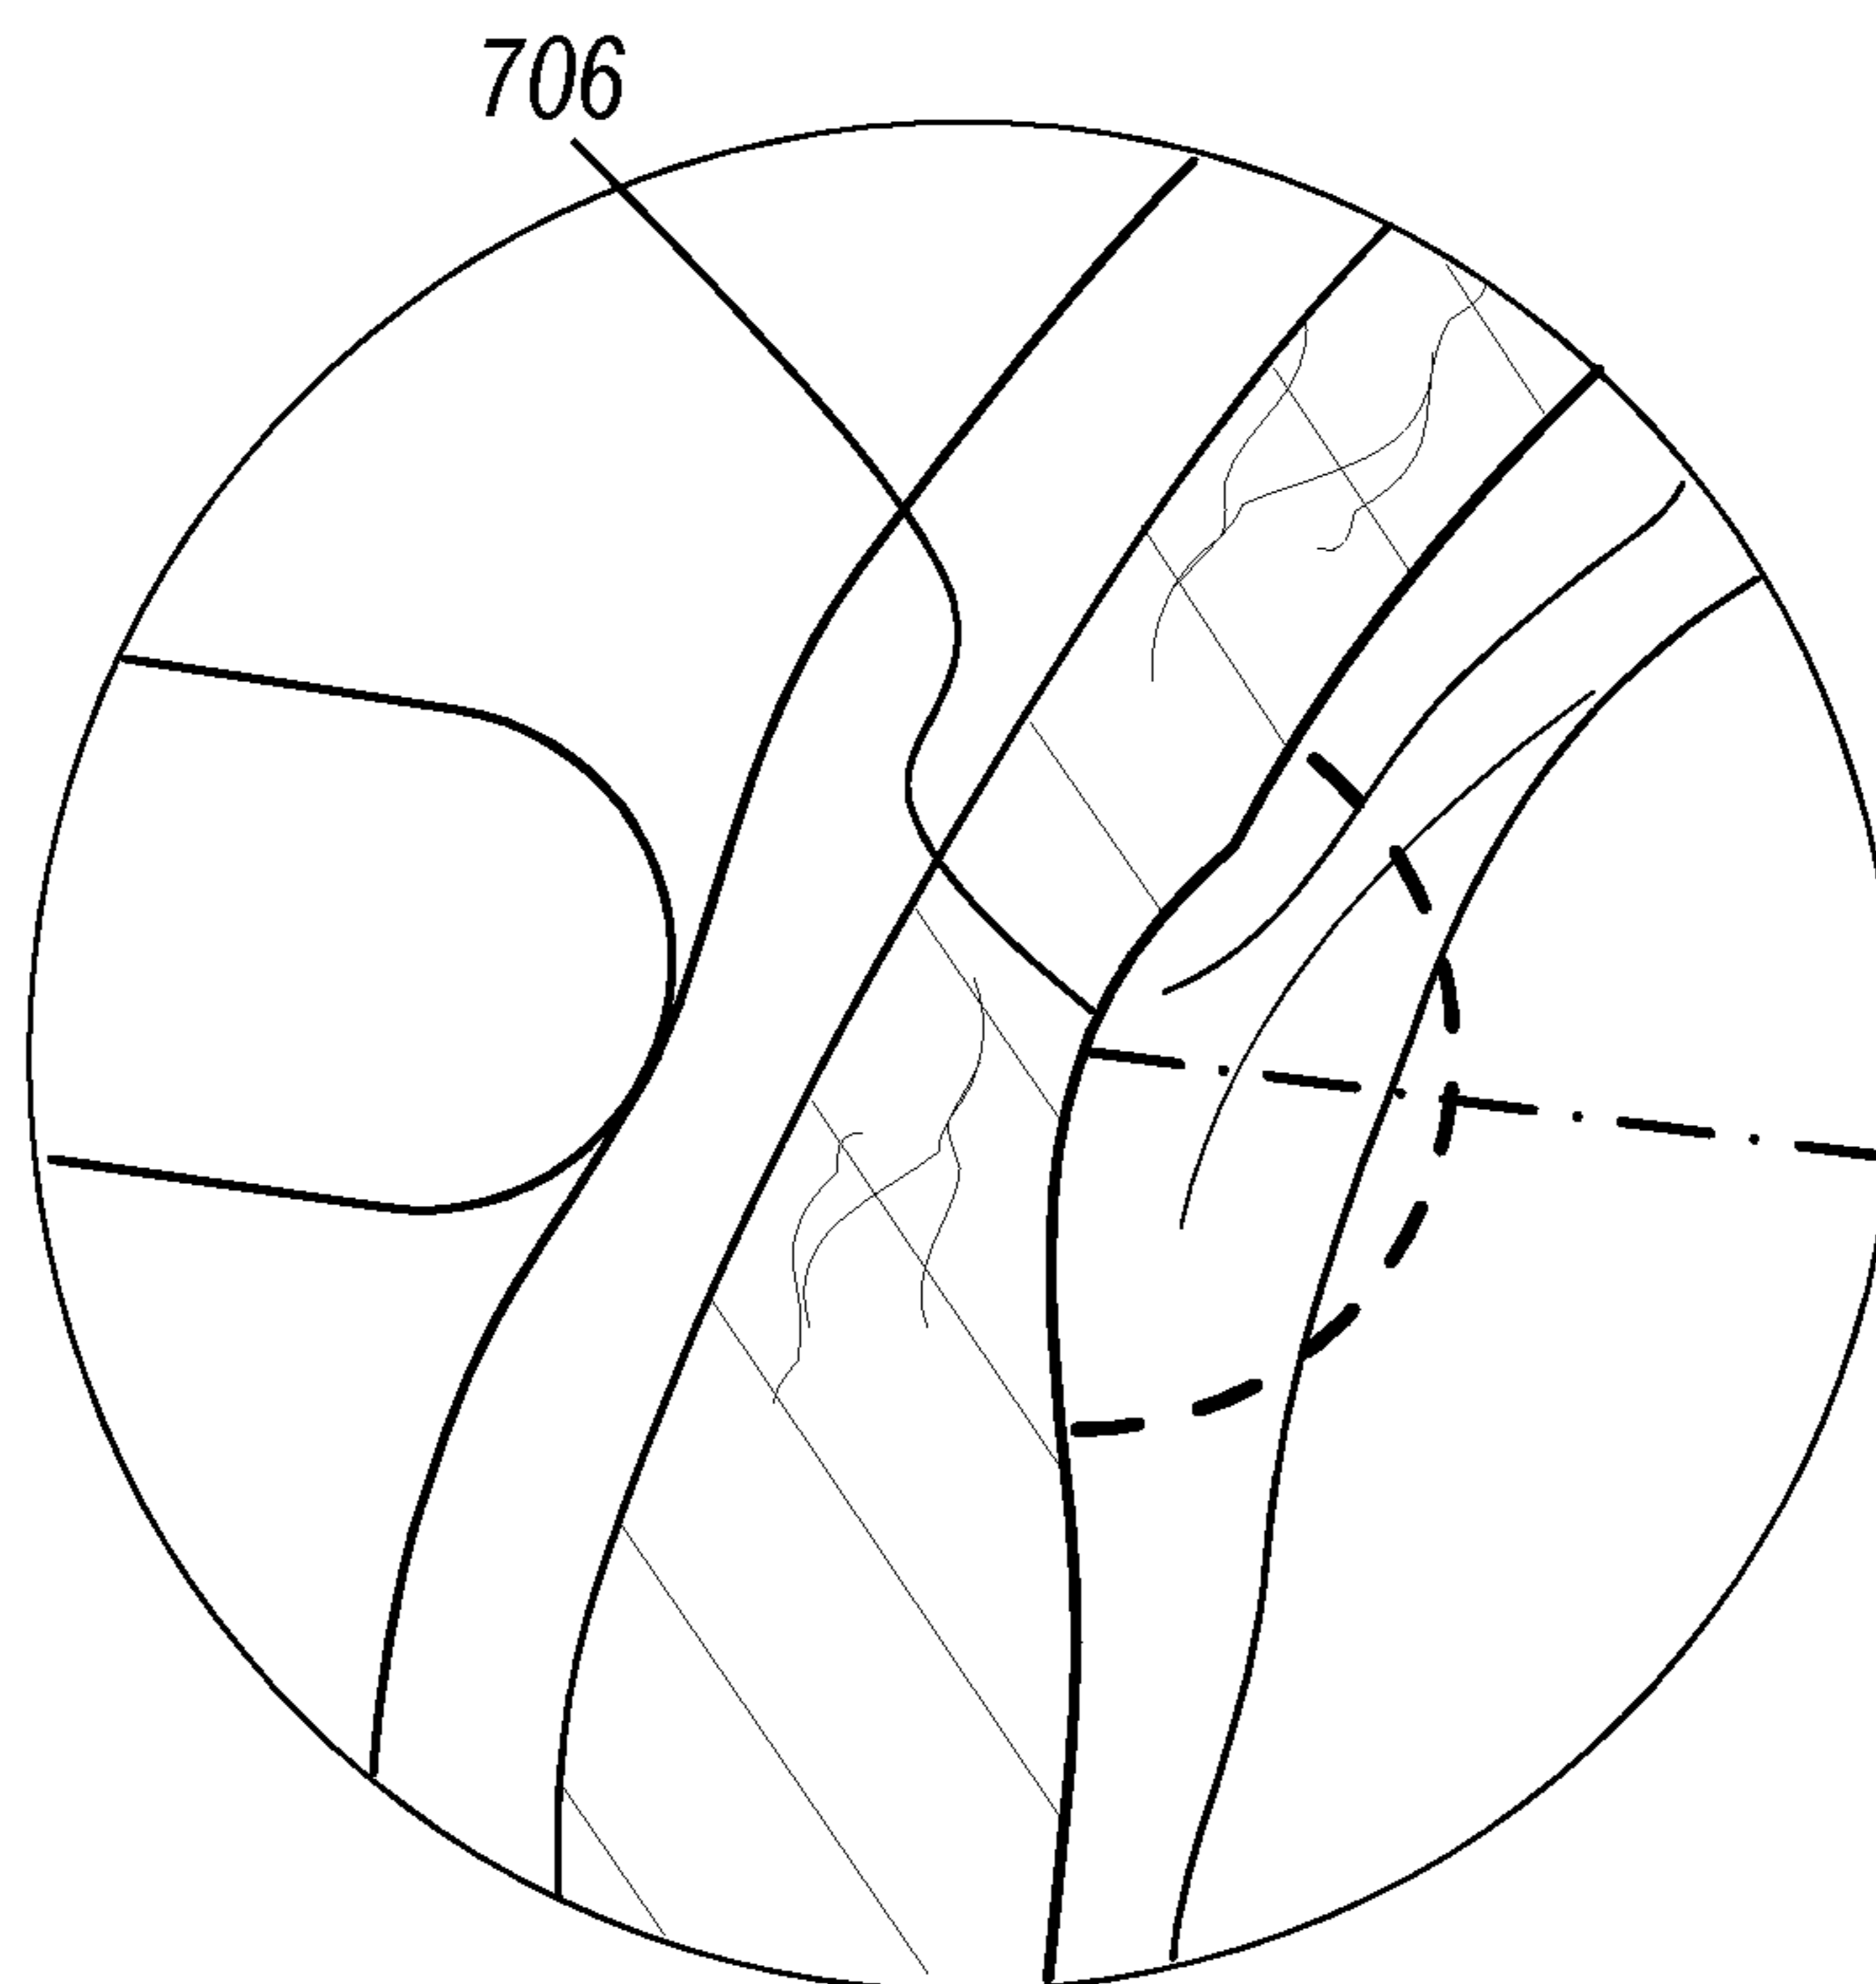


FIG. 34B

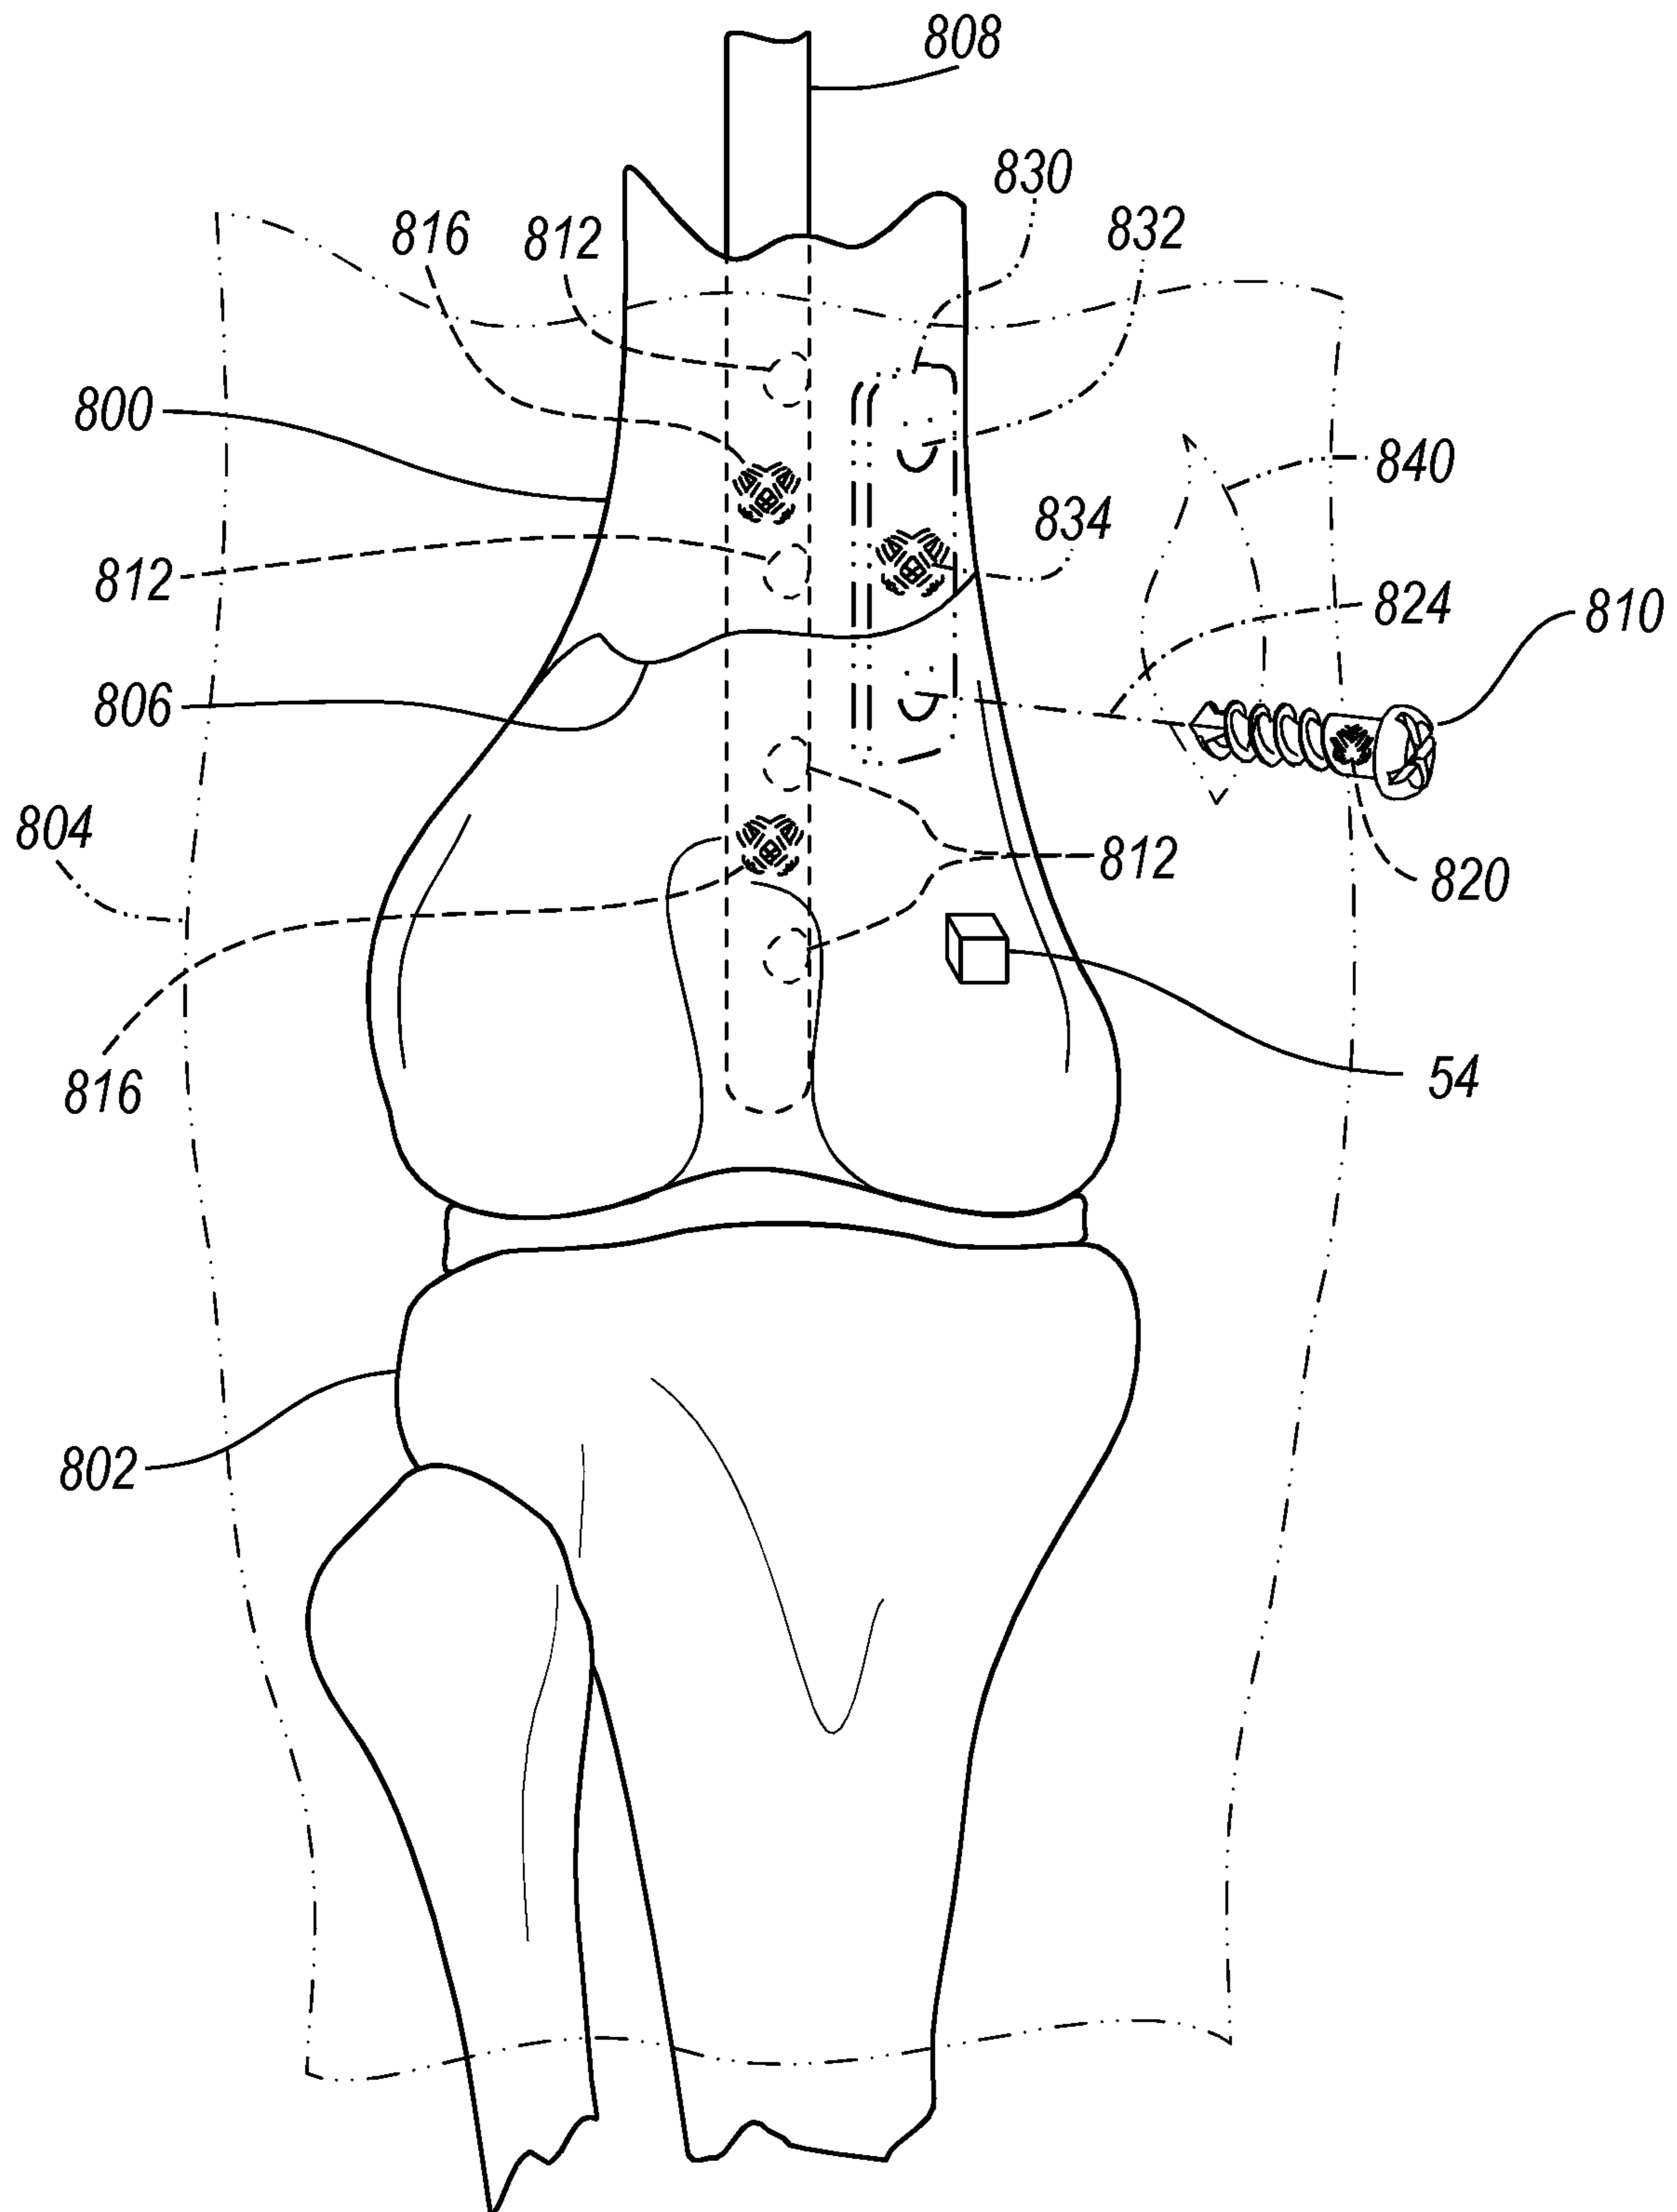


FIG. 35

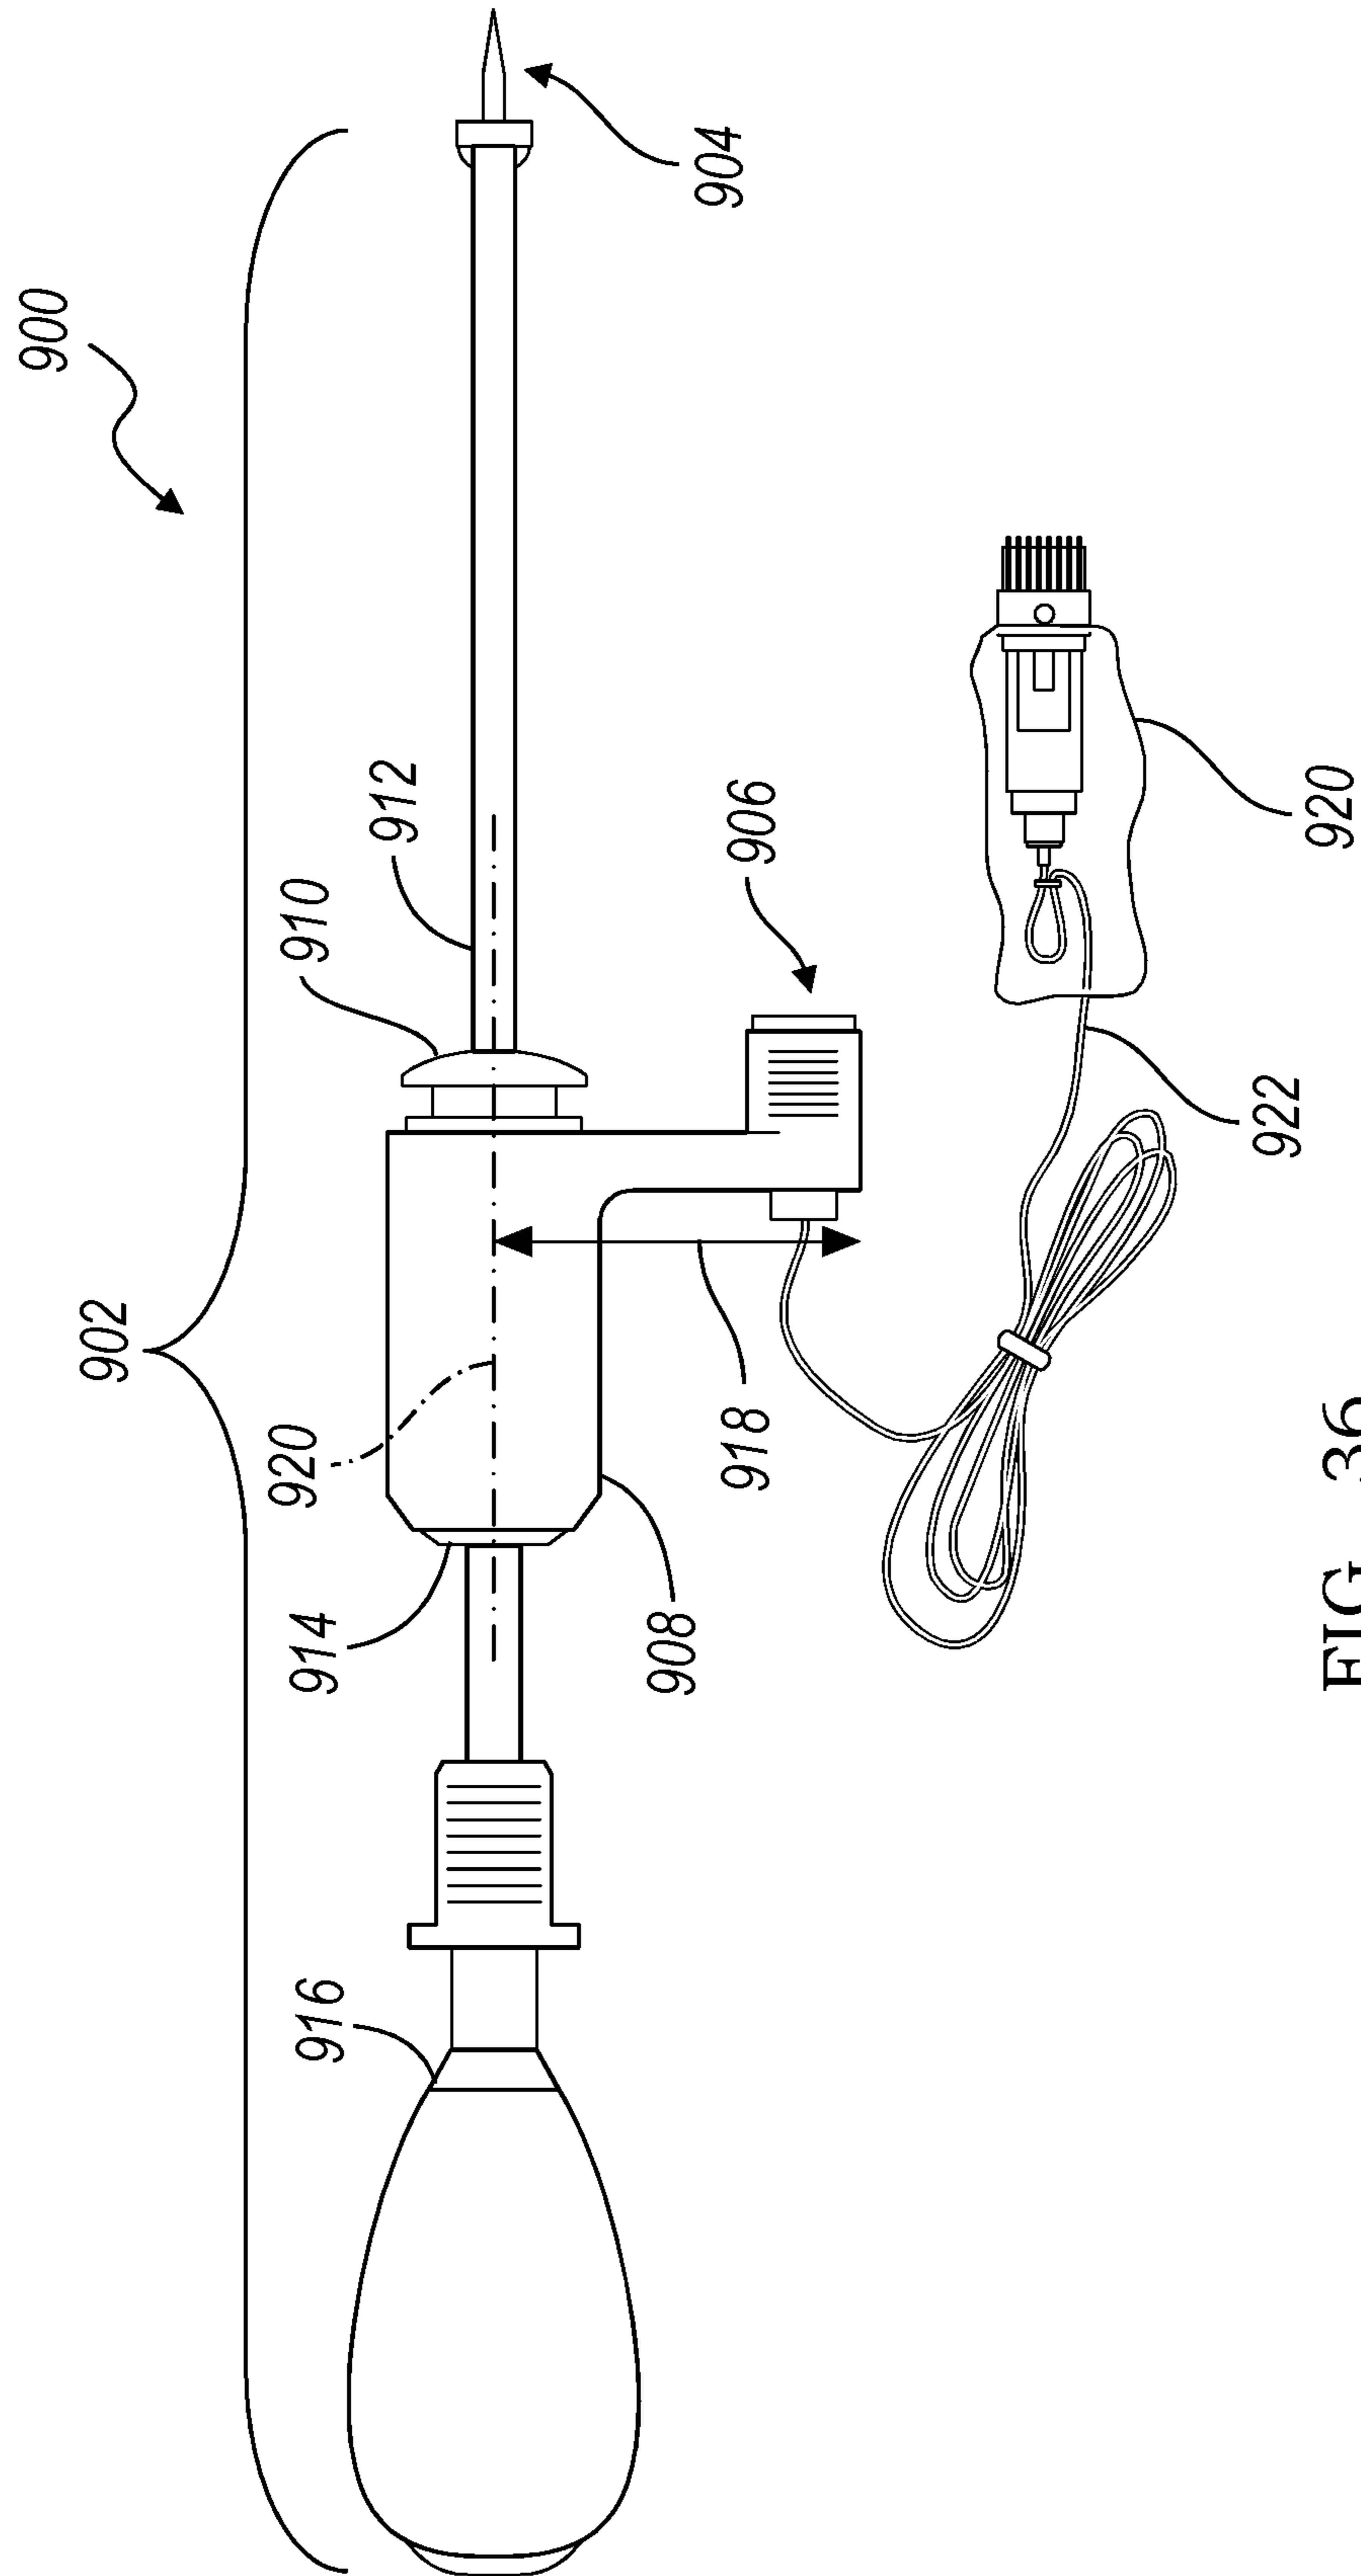


FIG. 36

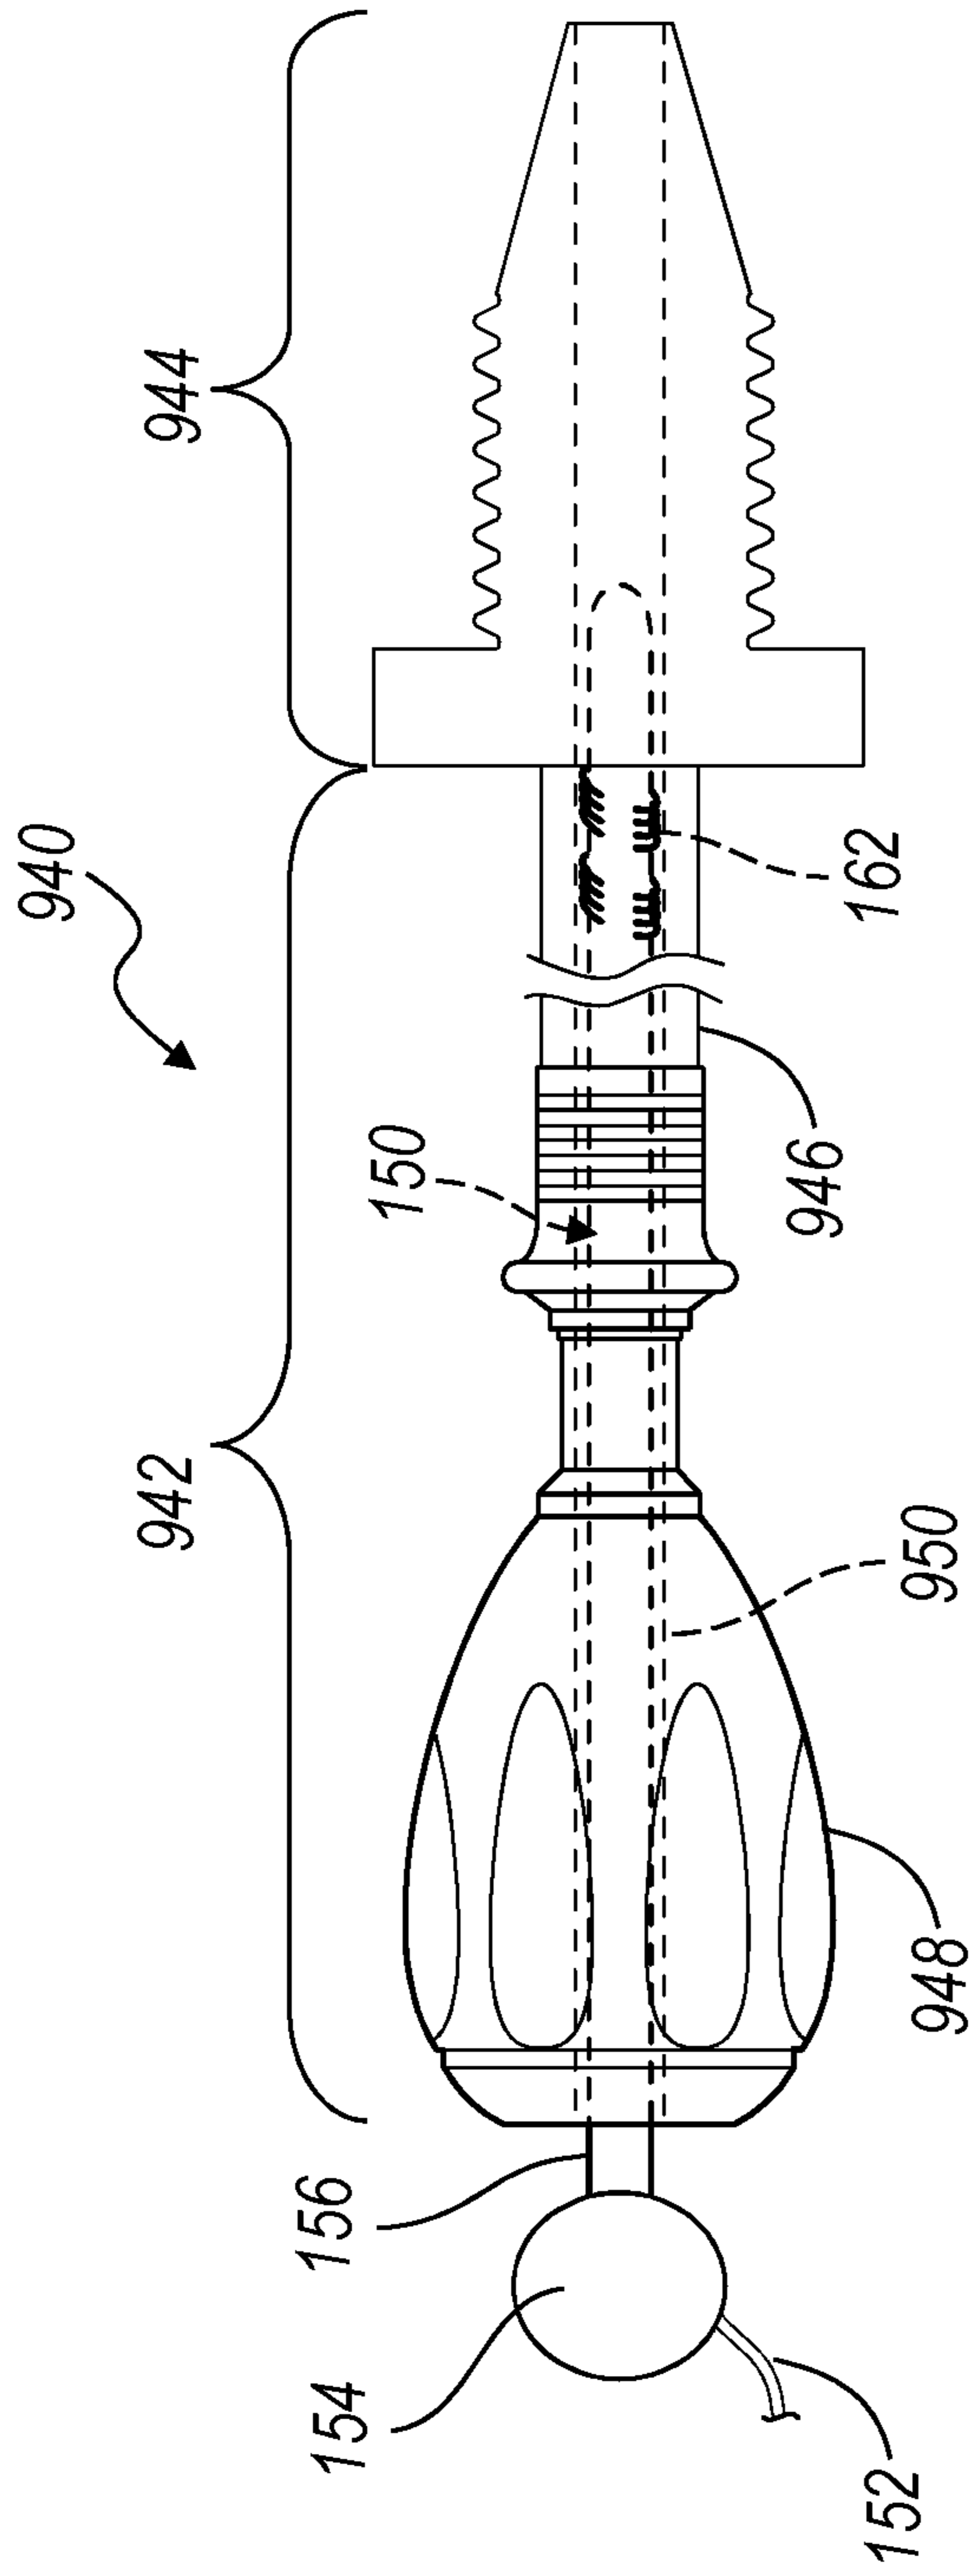


FIG. 37

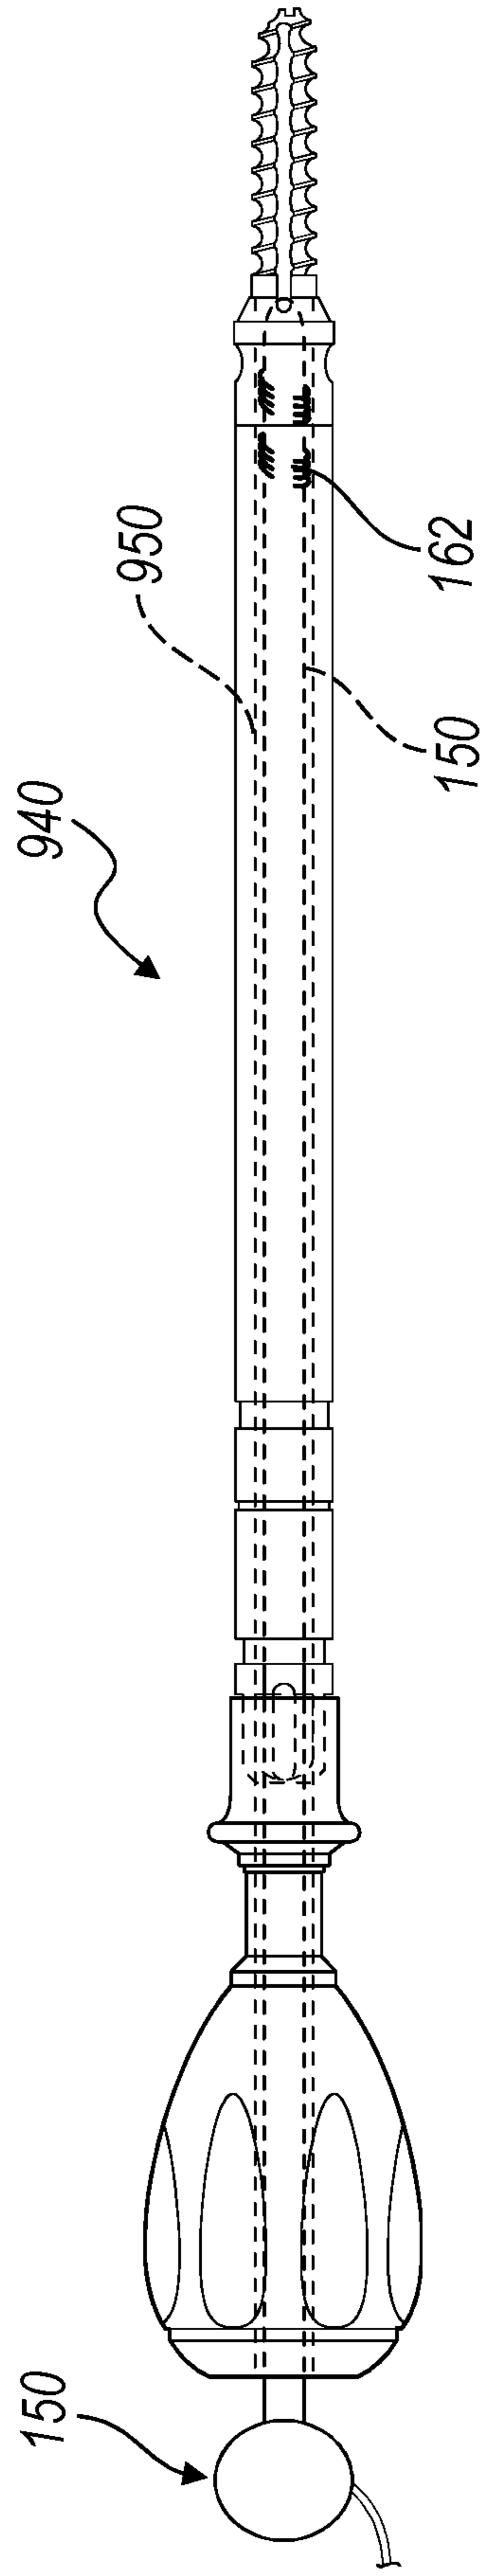


FIG. 38

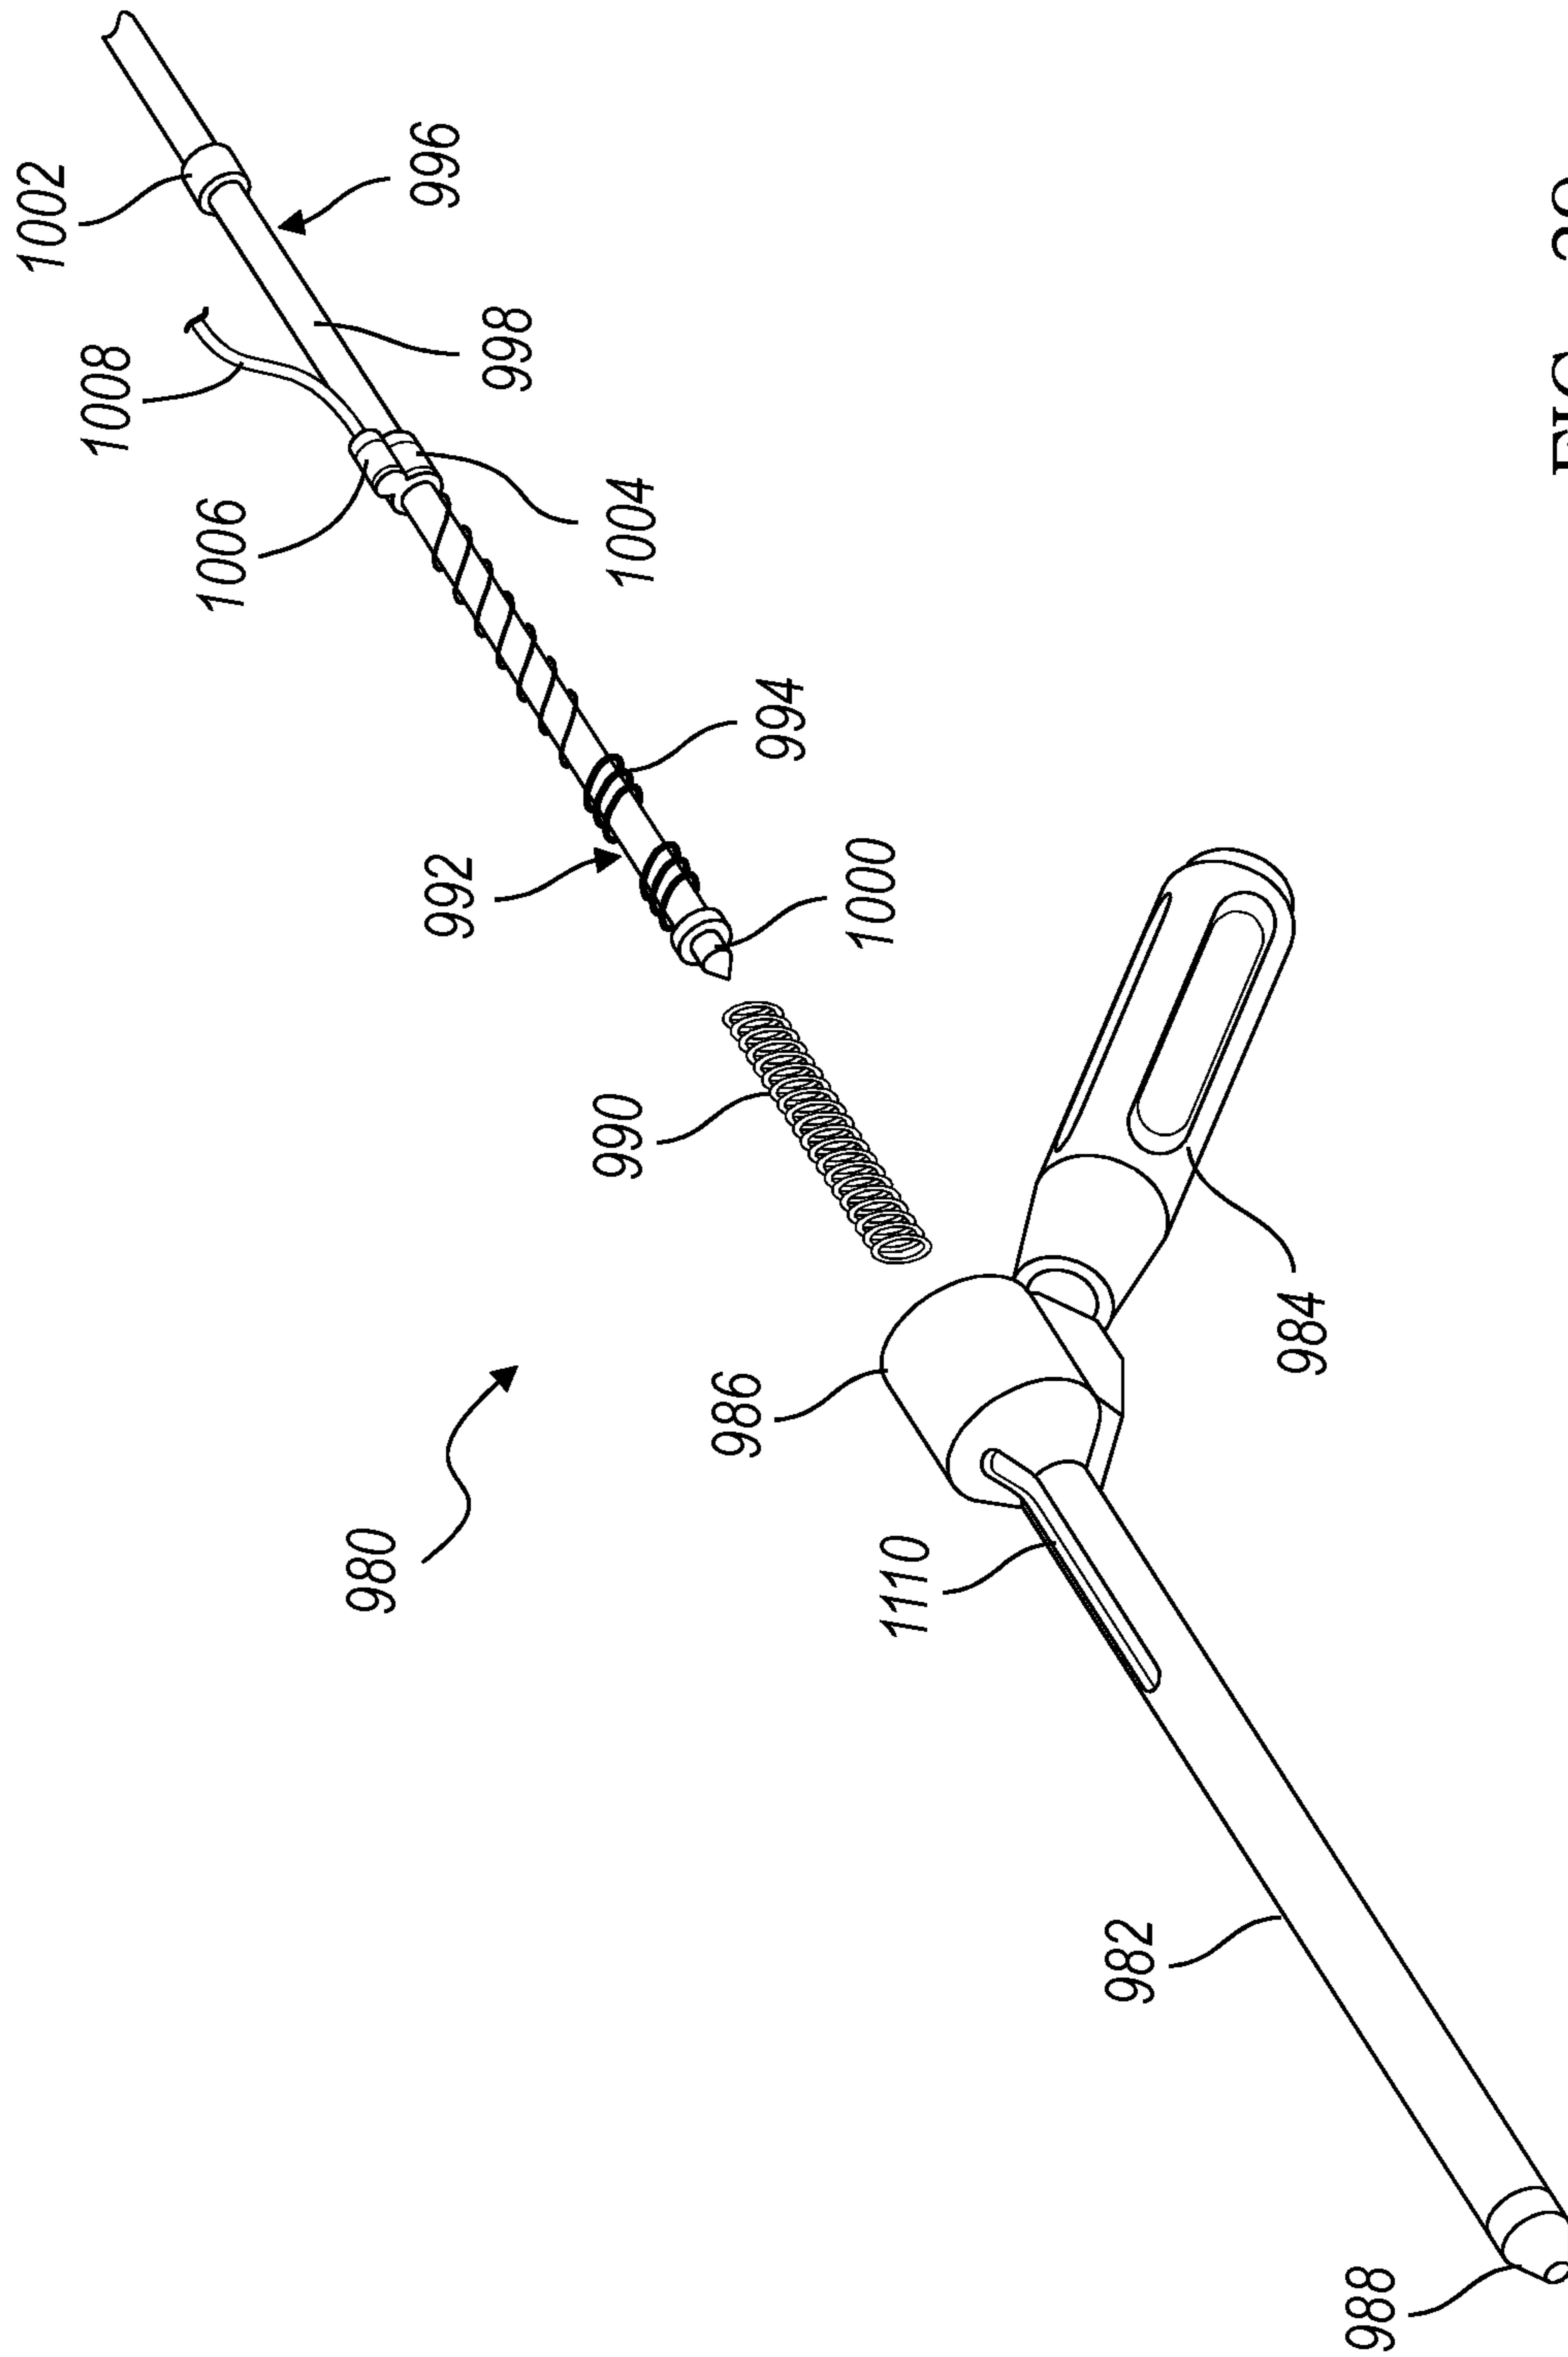


FIG. 39

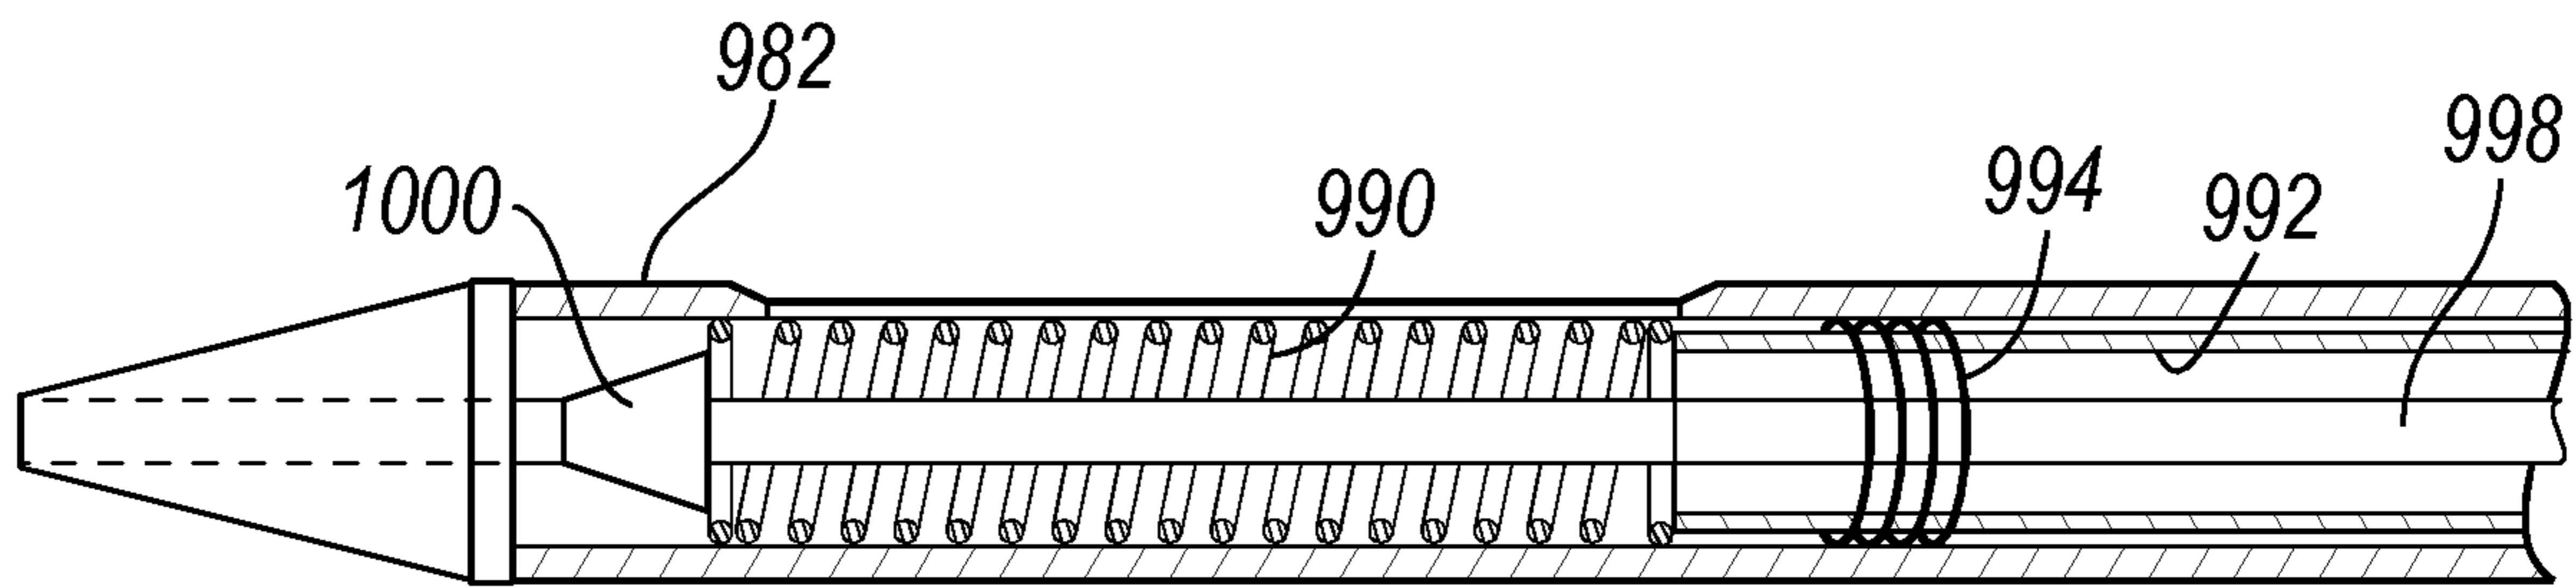


FIG. 40

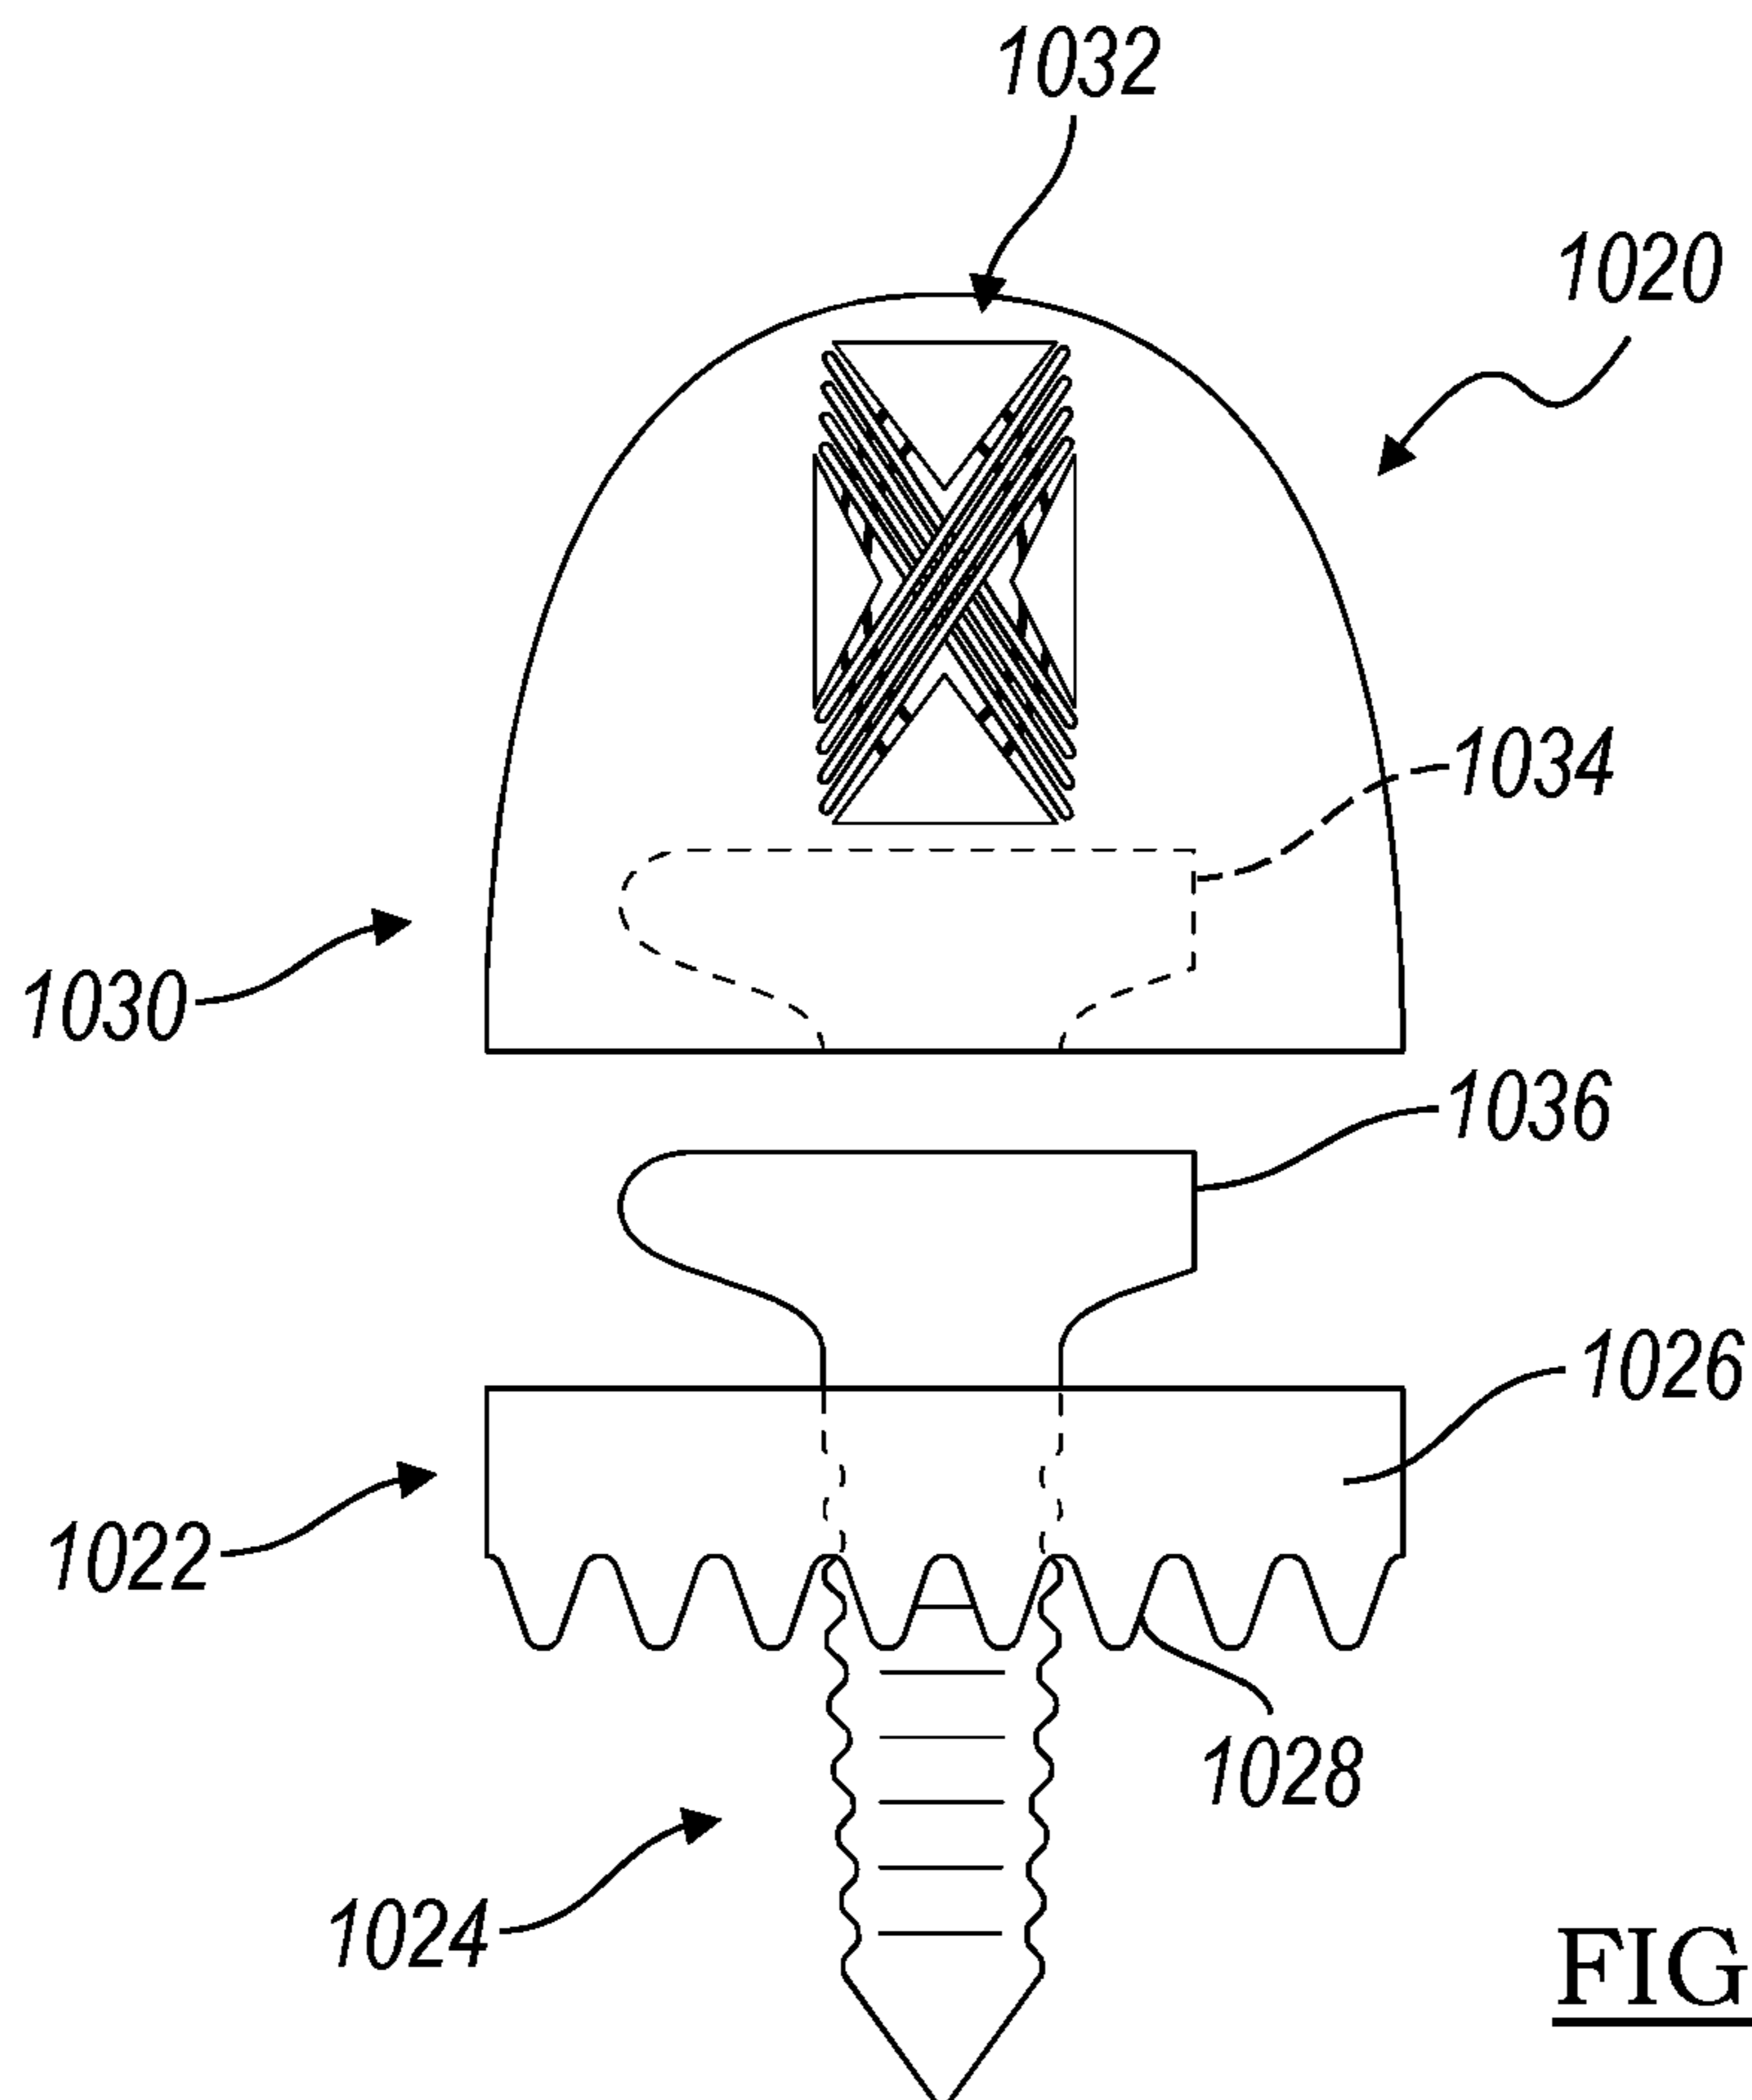


FIG. 41

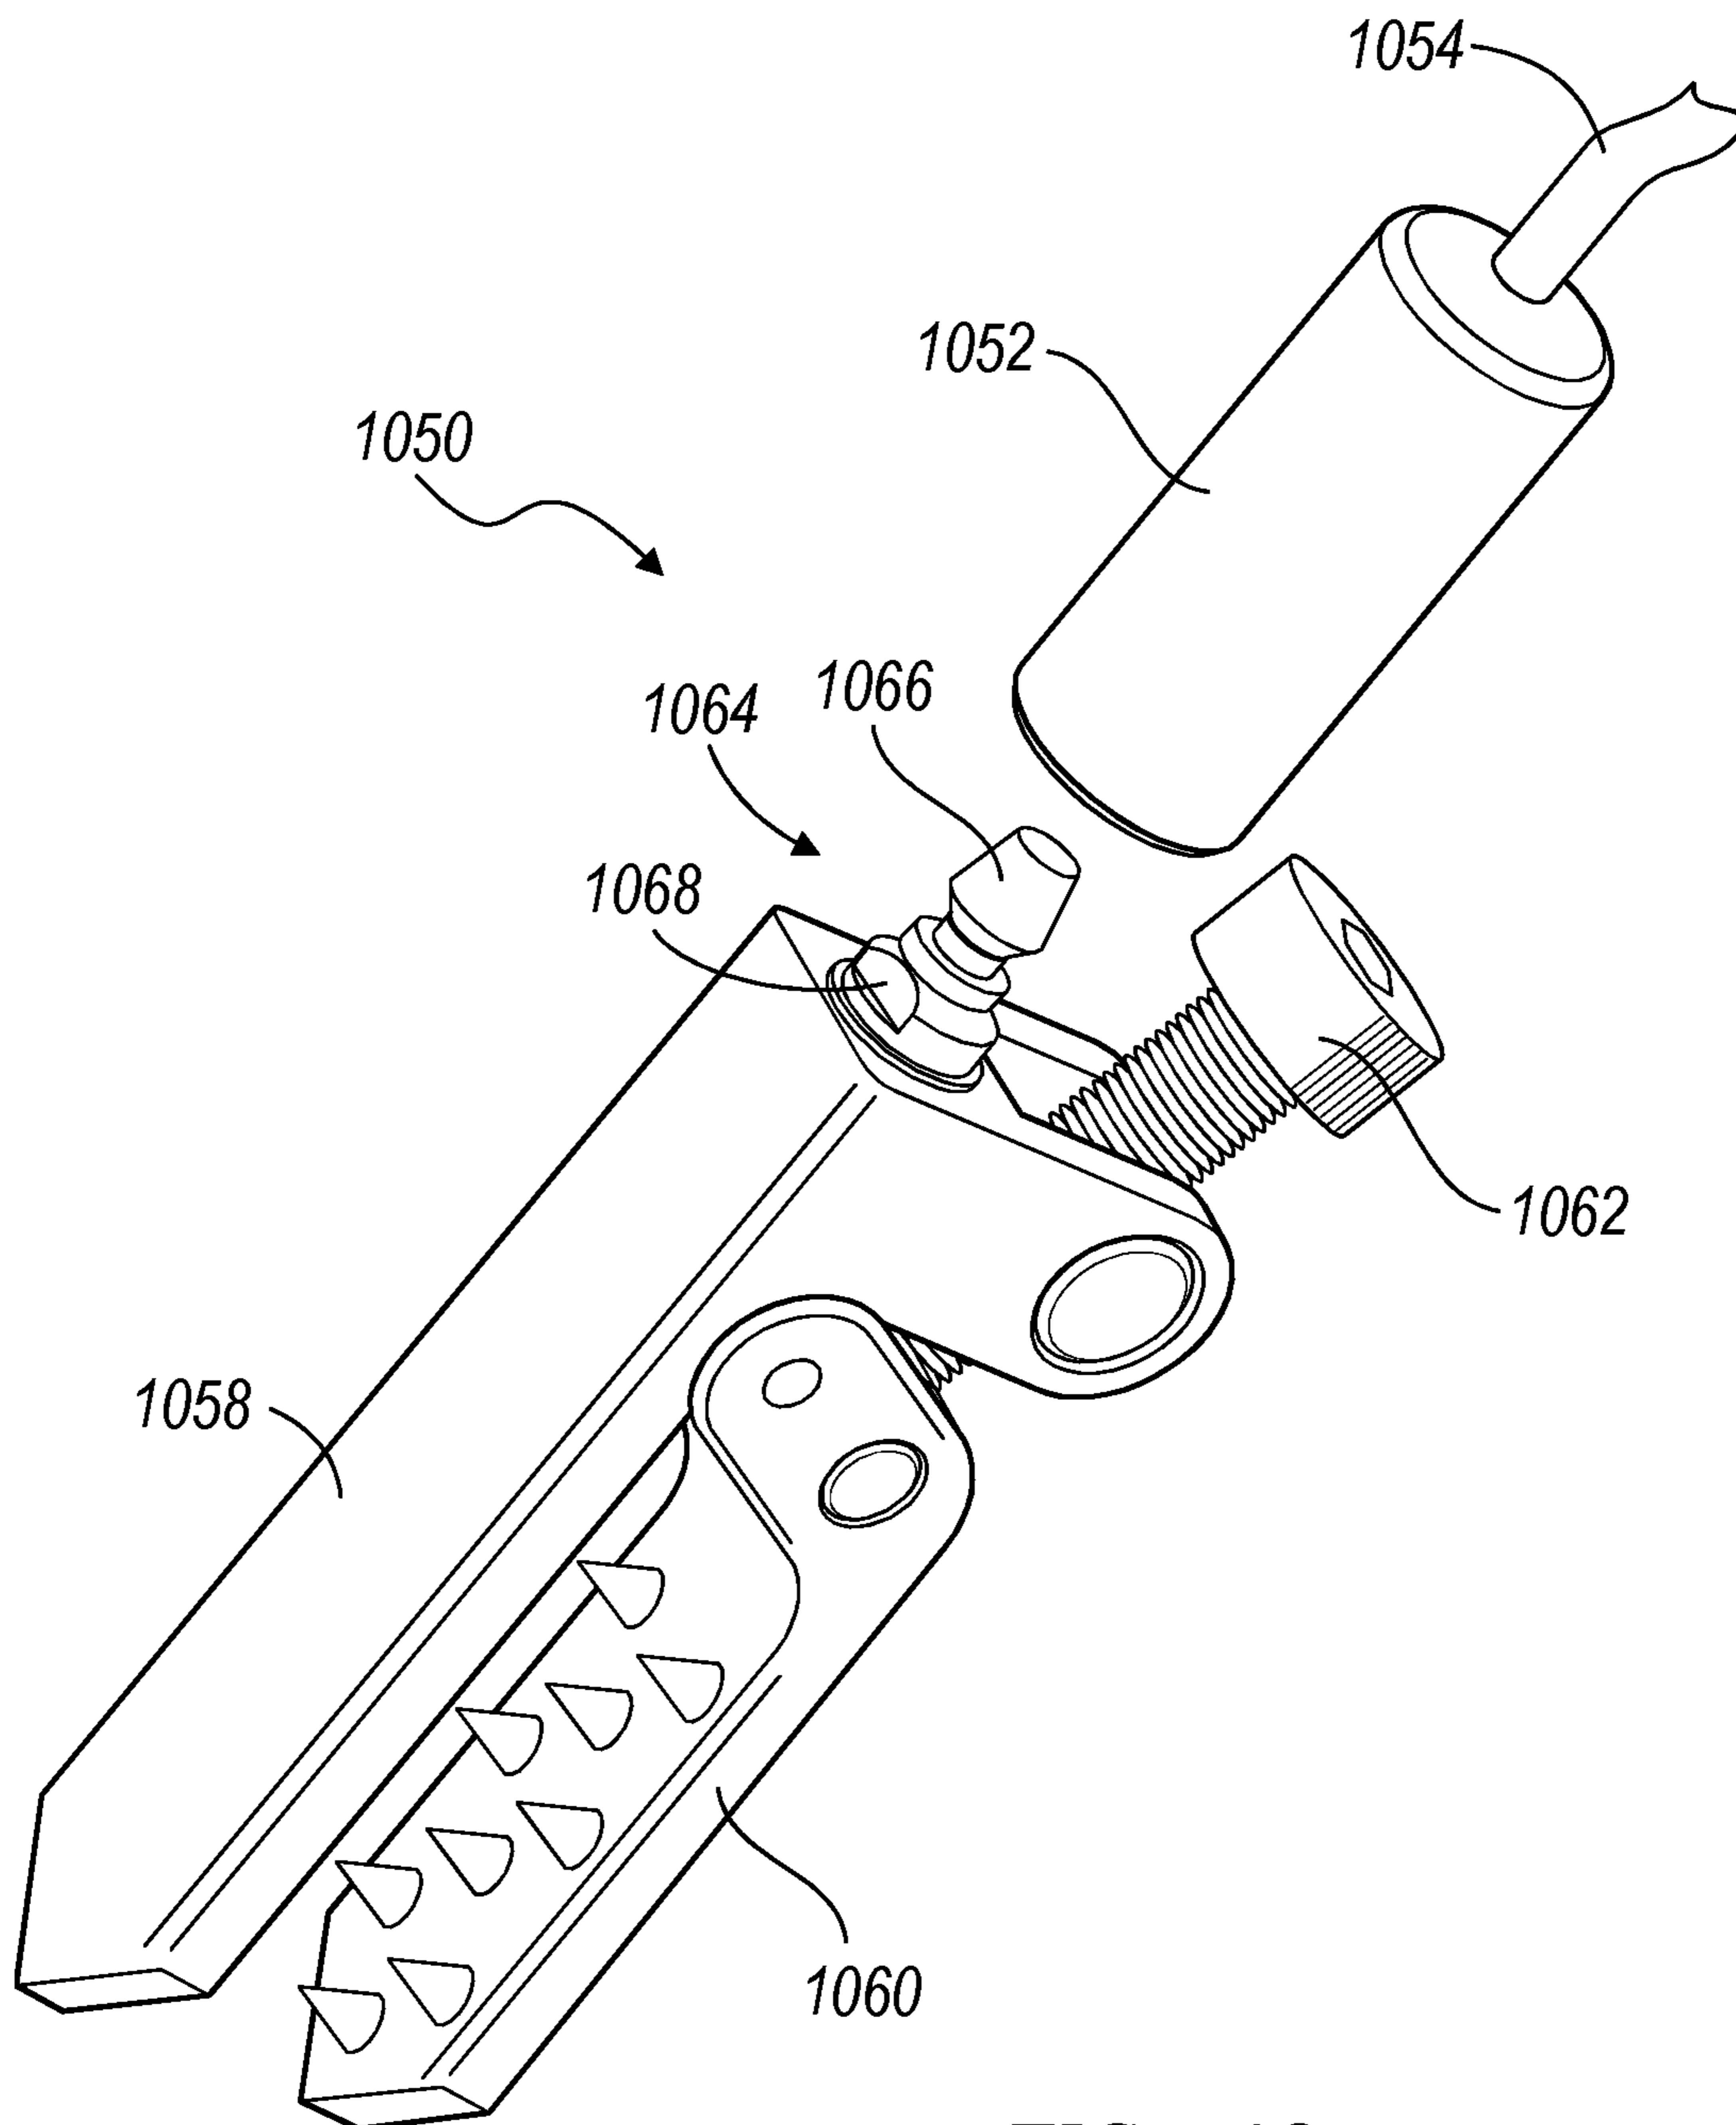


FIG. 42

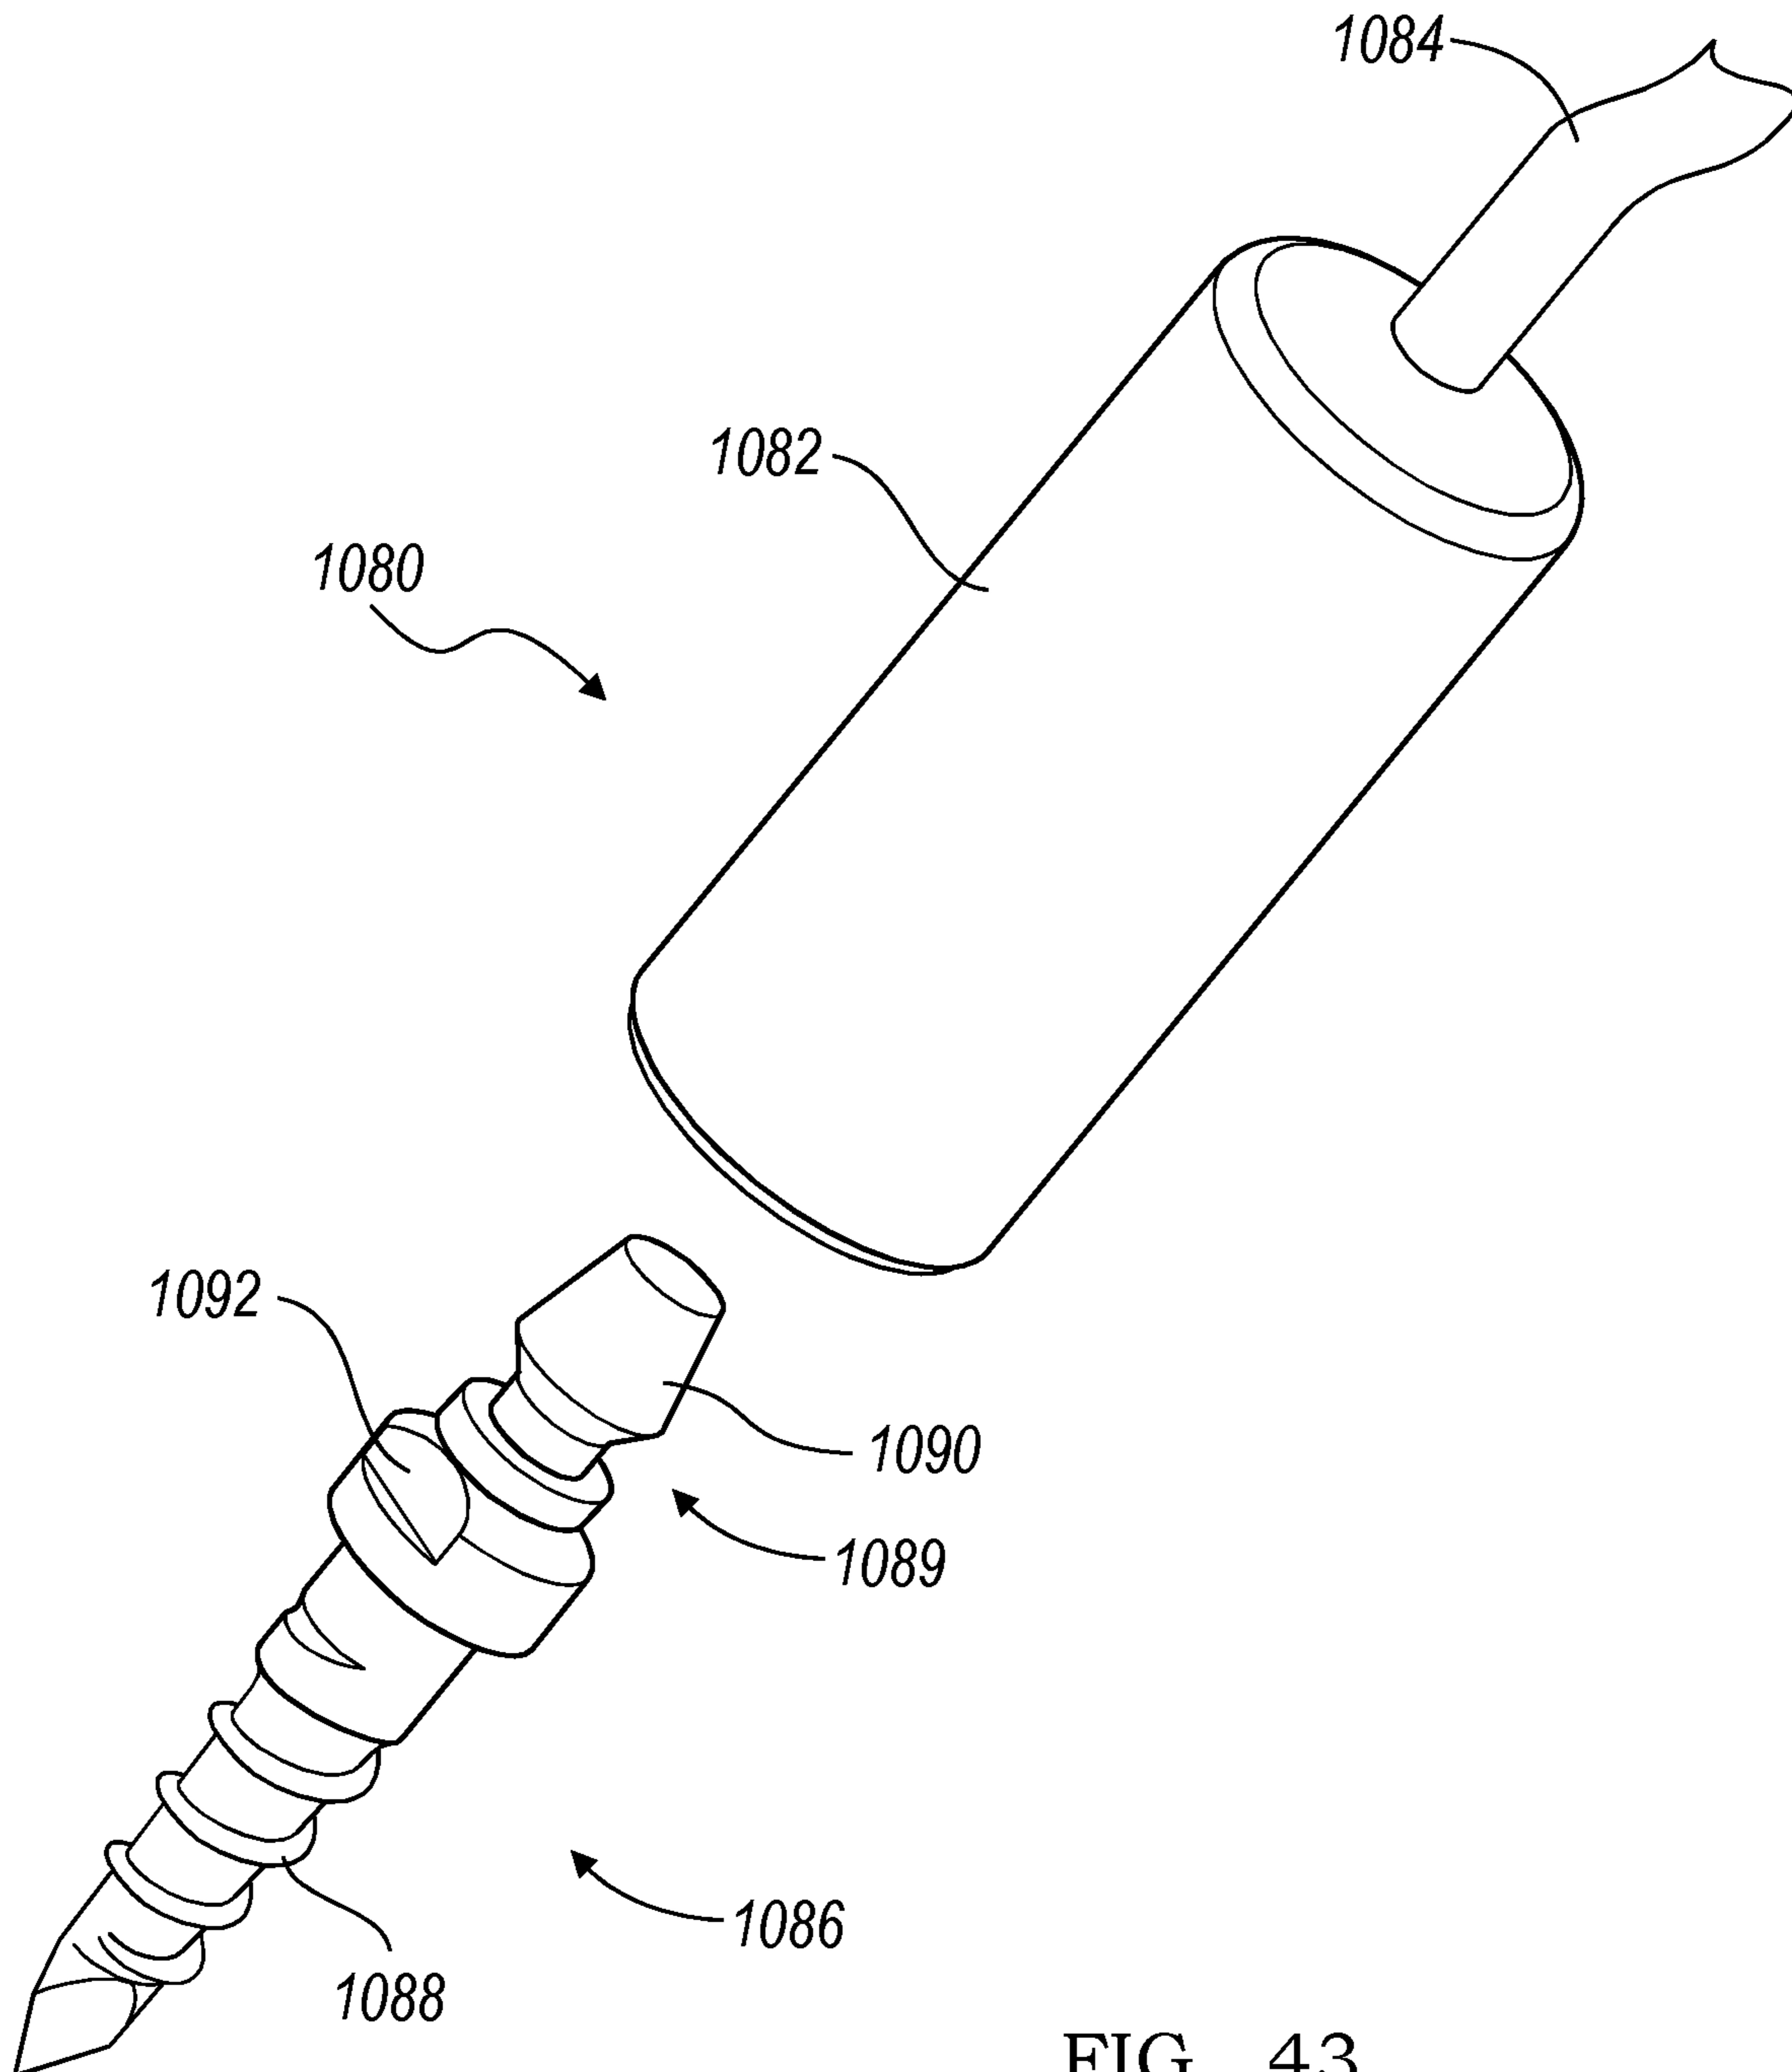


FIG. 43

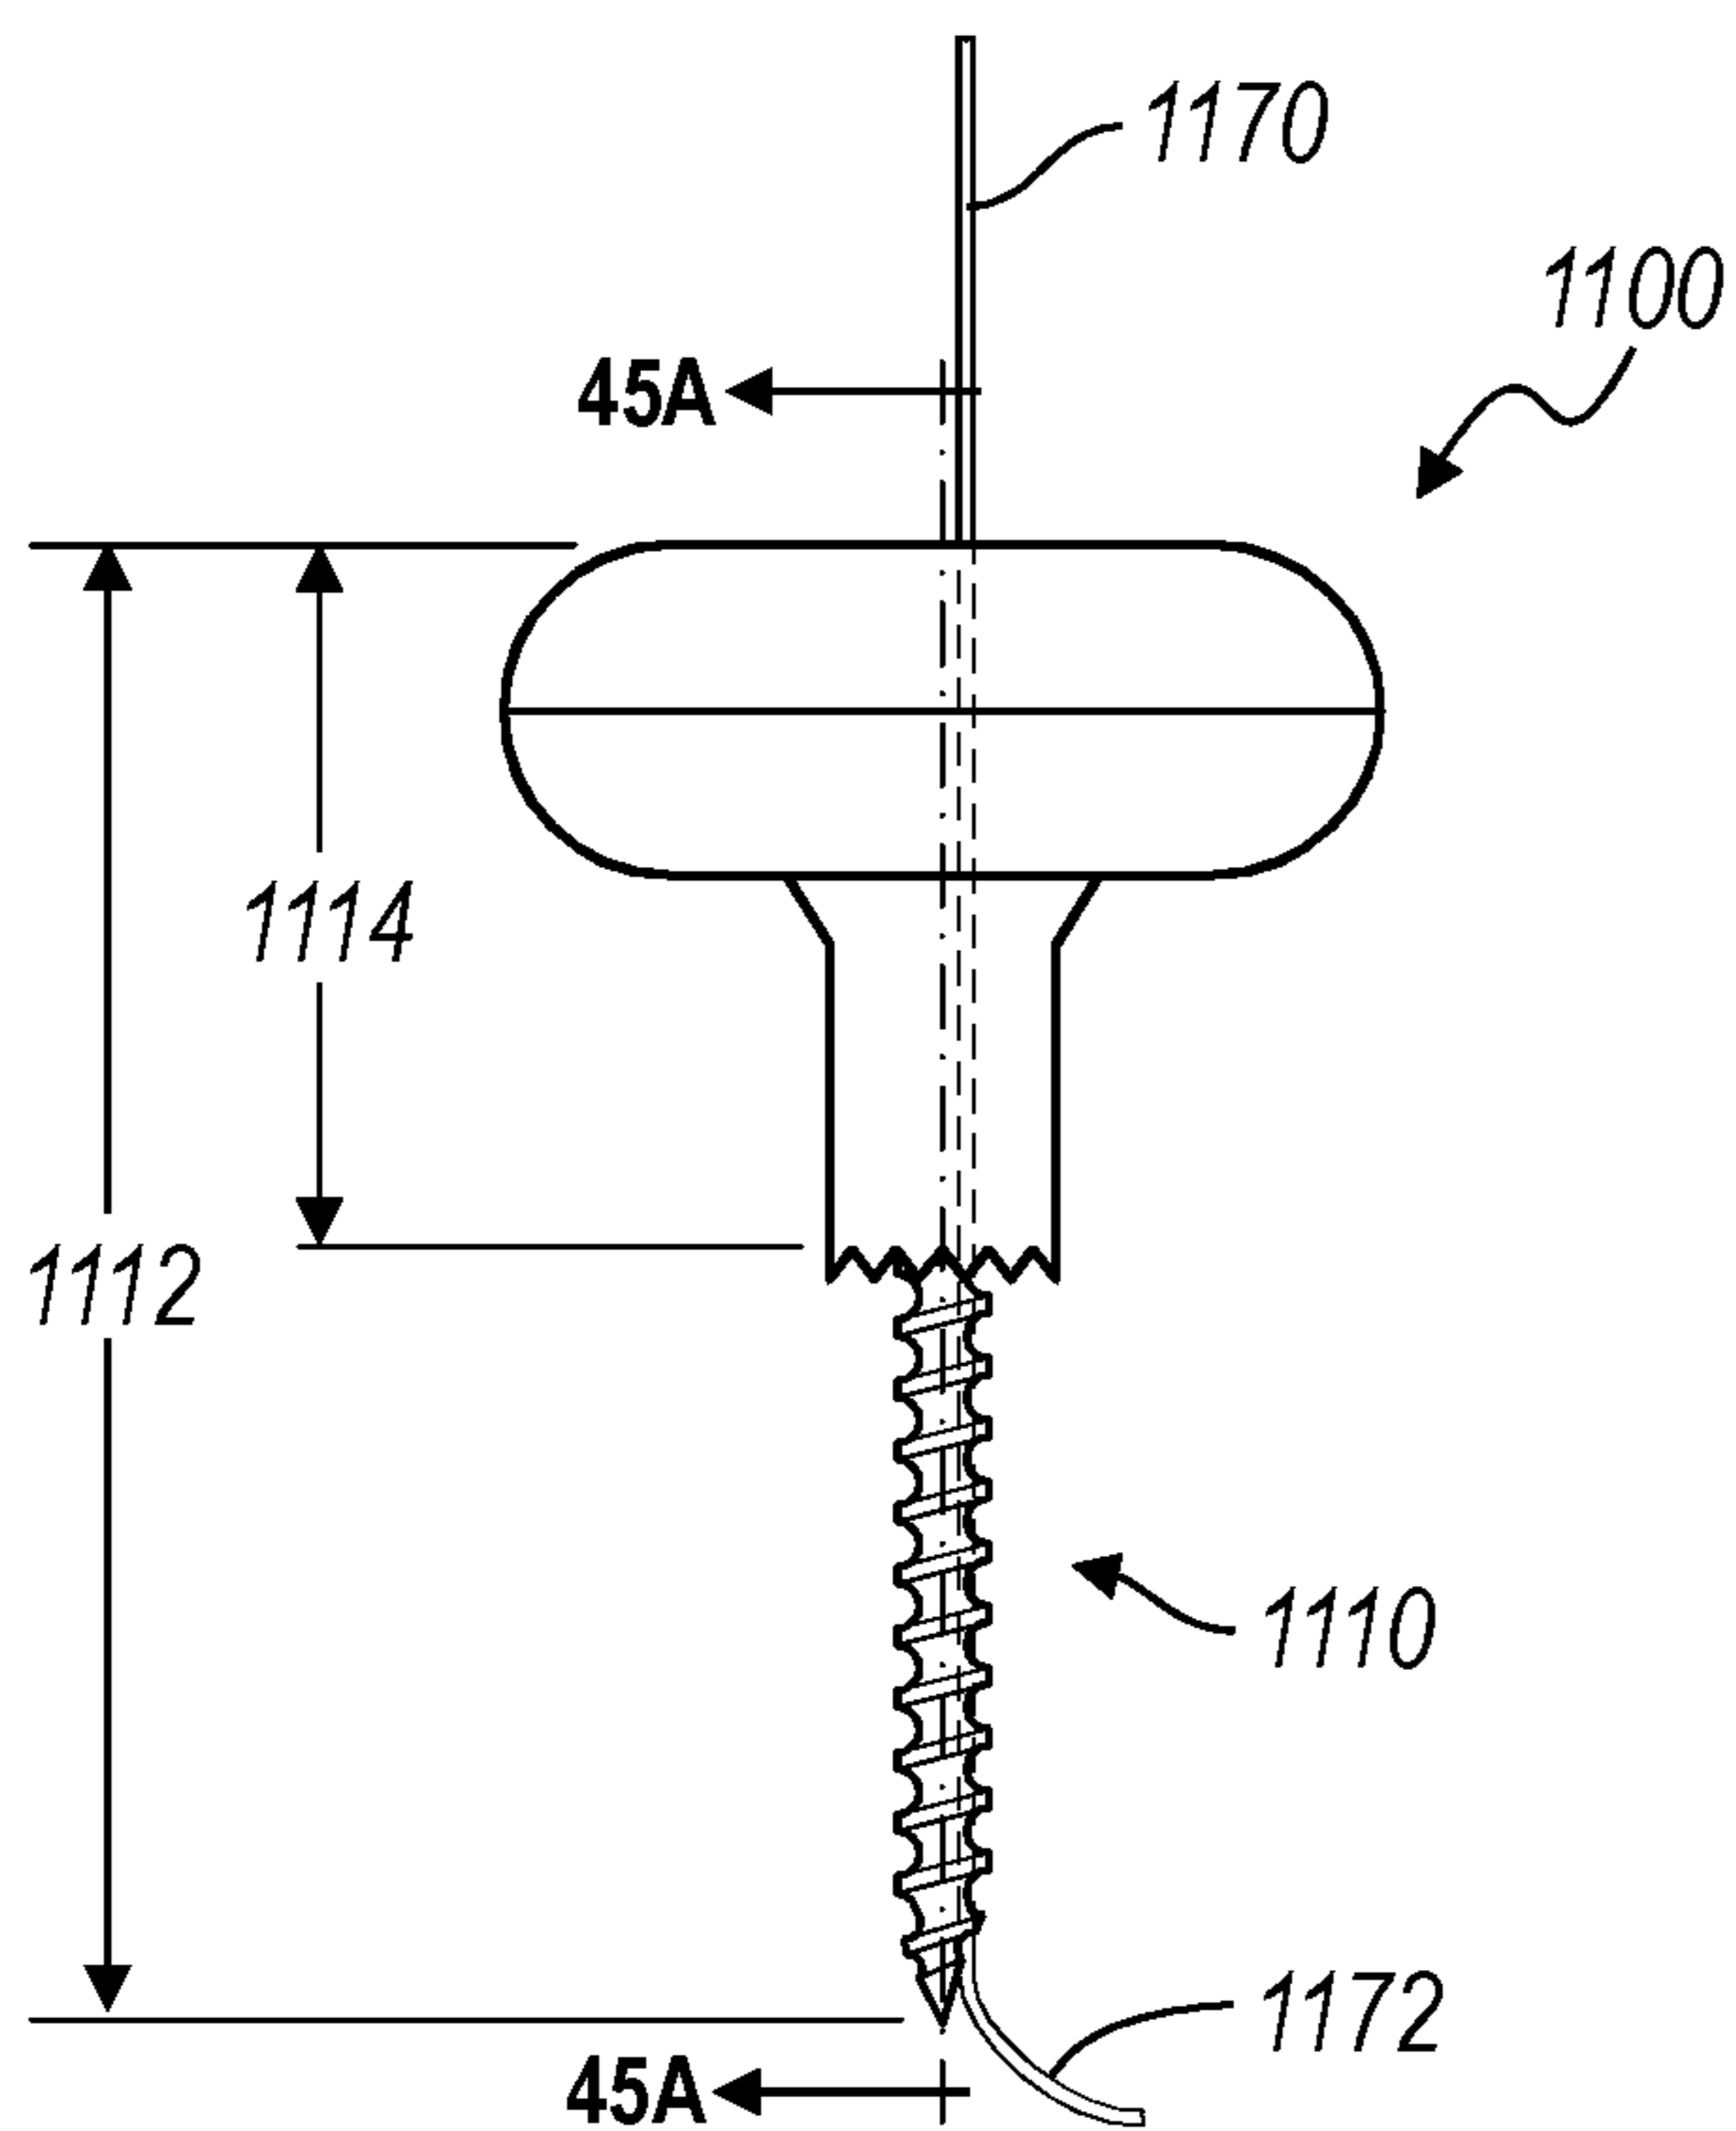


FIG. 44

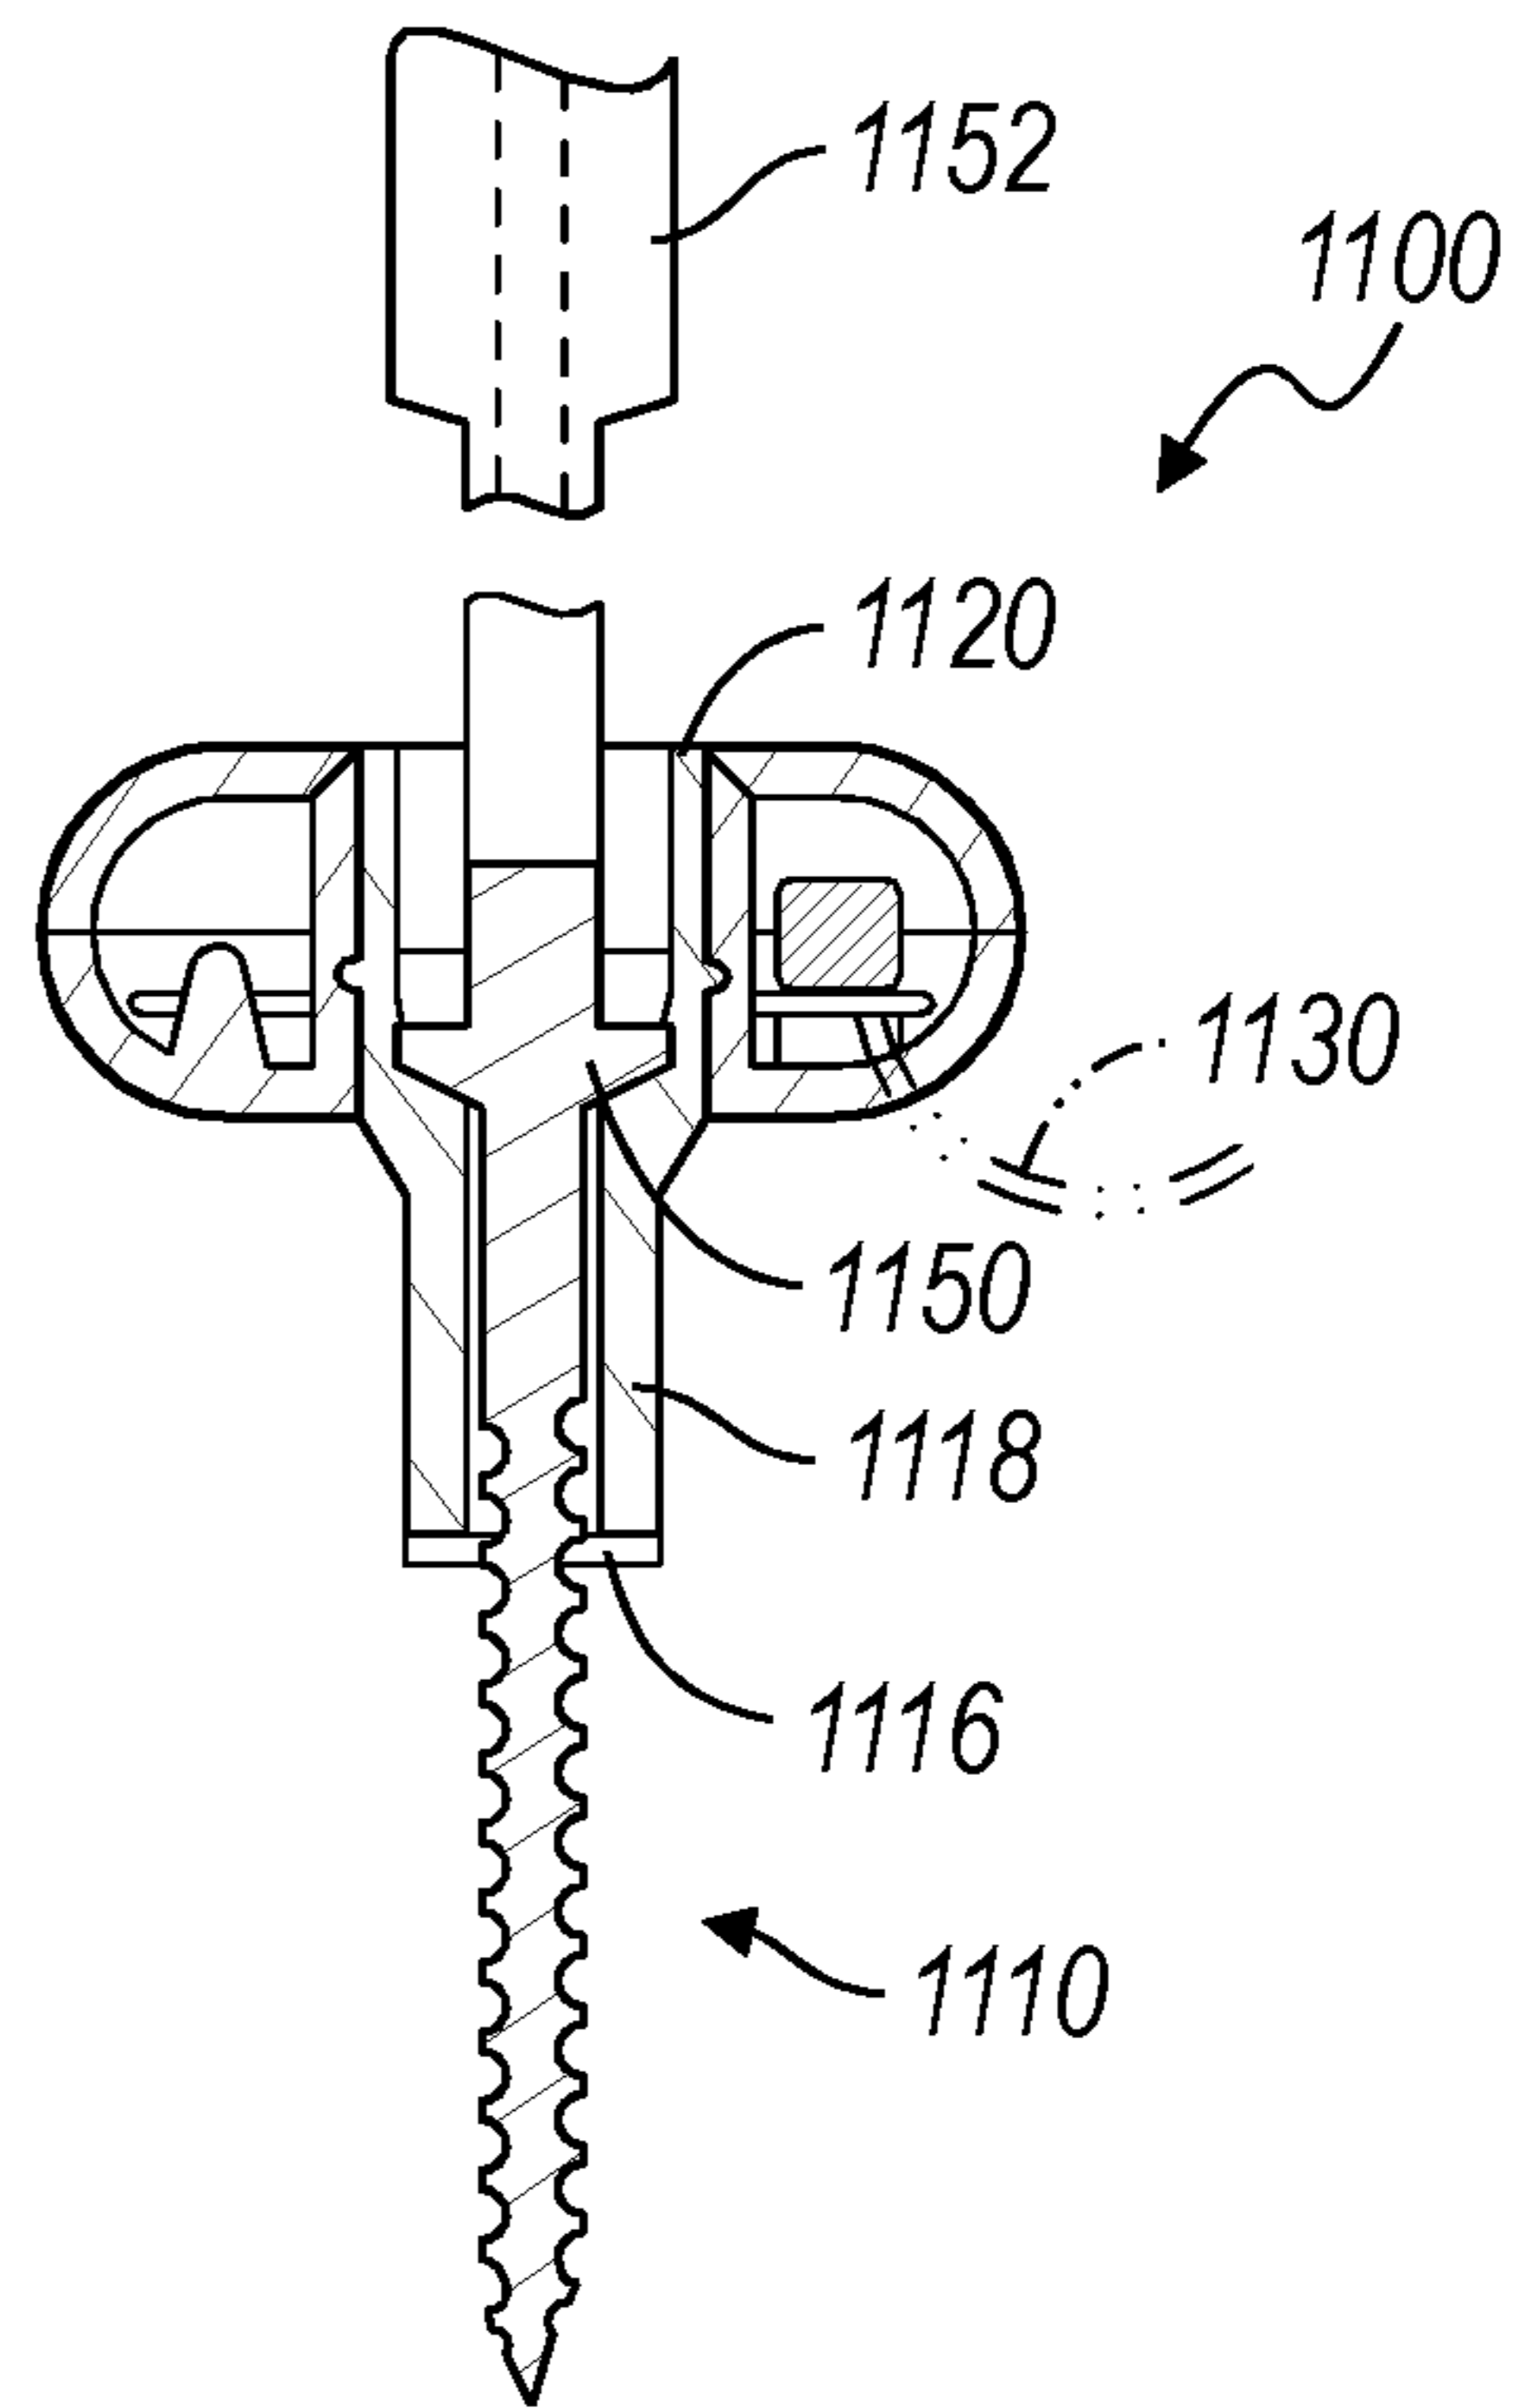


FIG. 45A

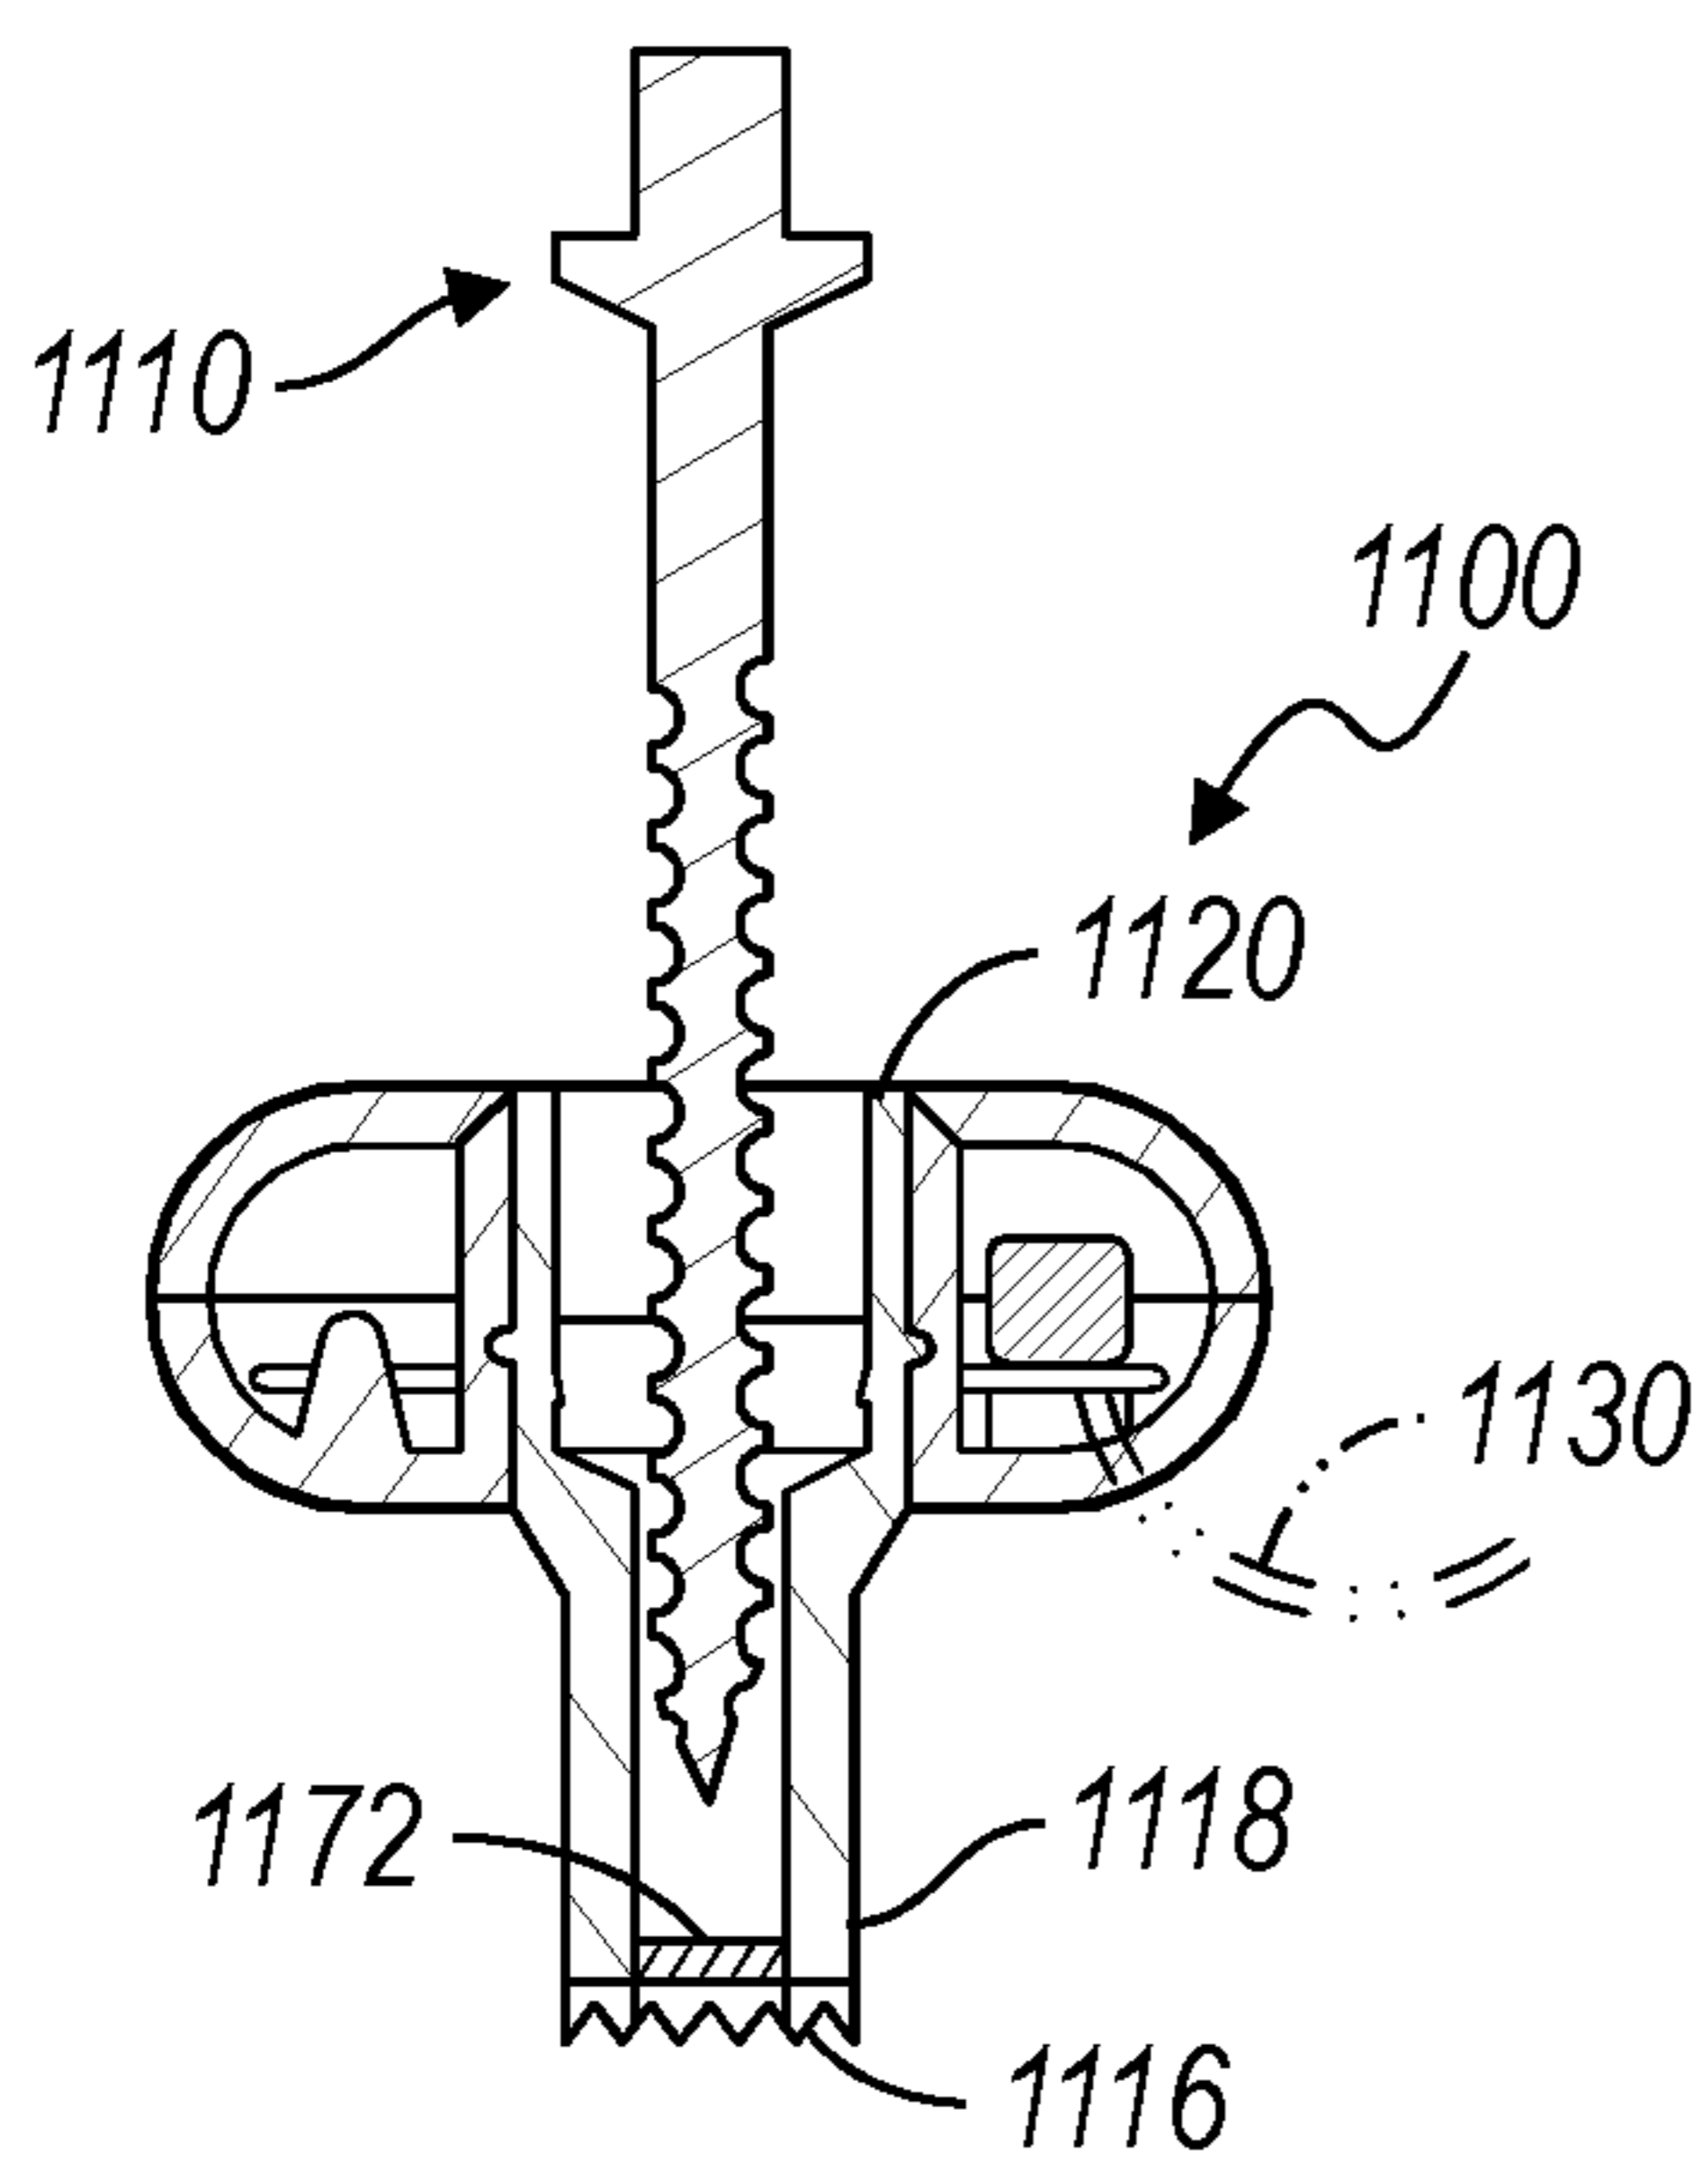


FIG. 45B

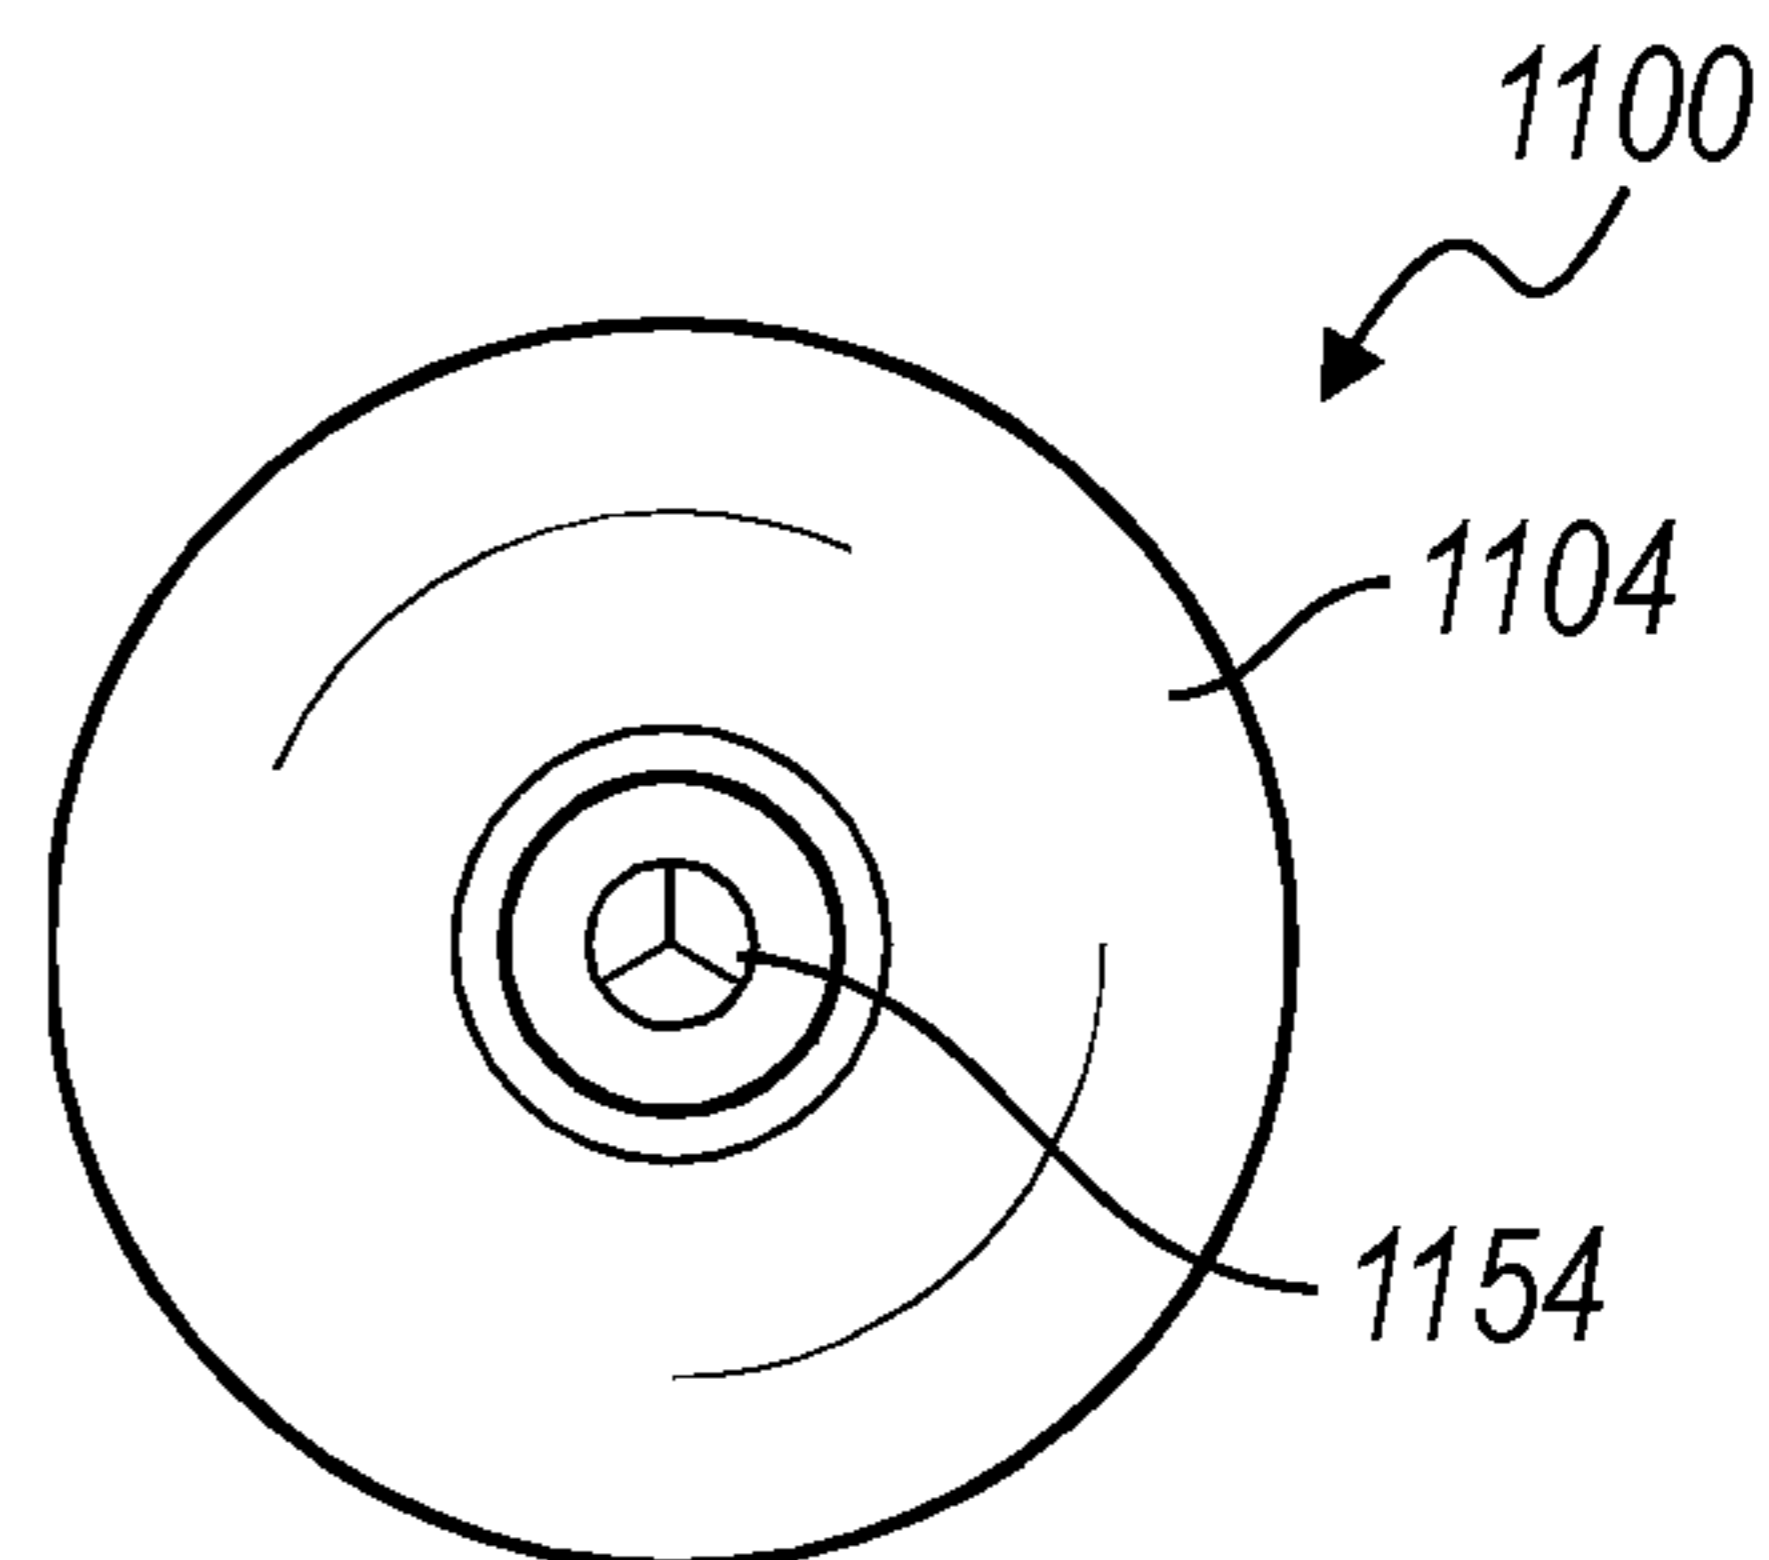


FIG. 46

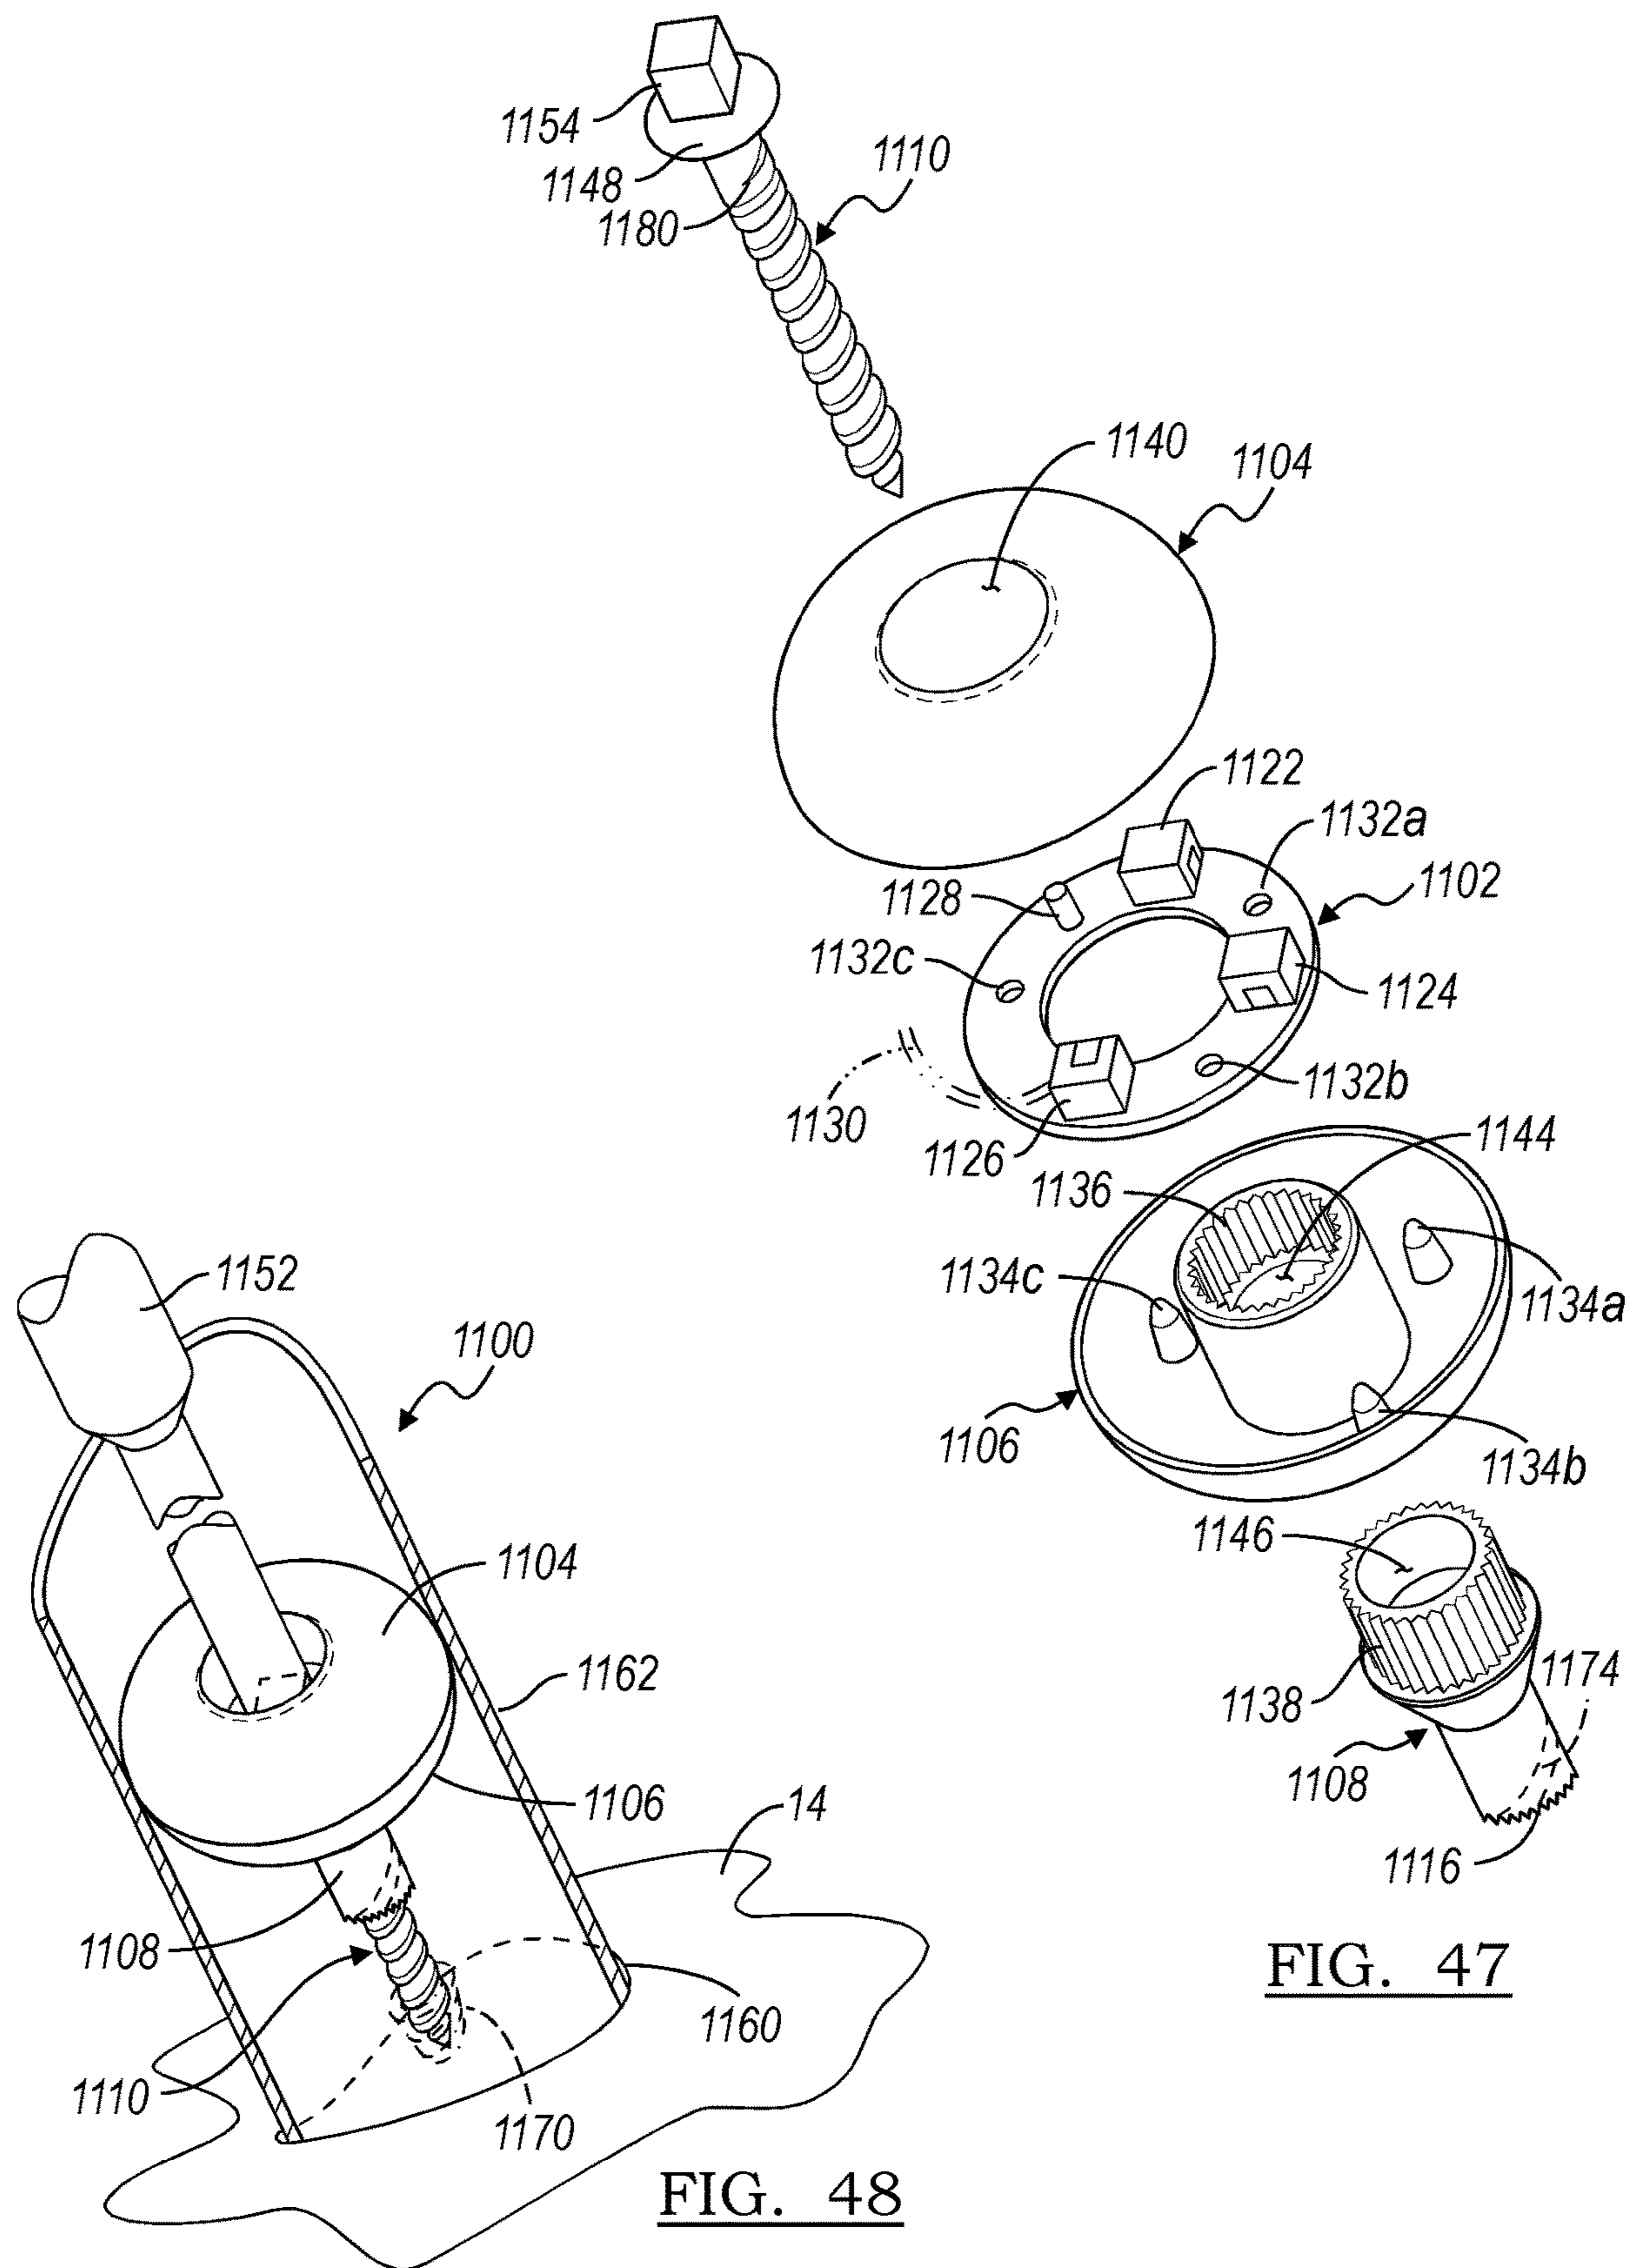


FIG. 48

FIG. 47

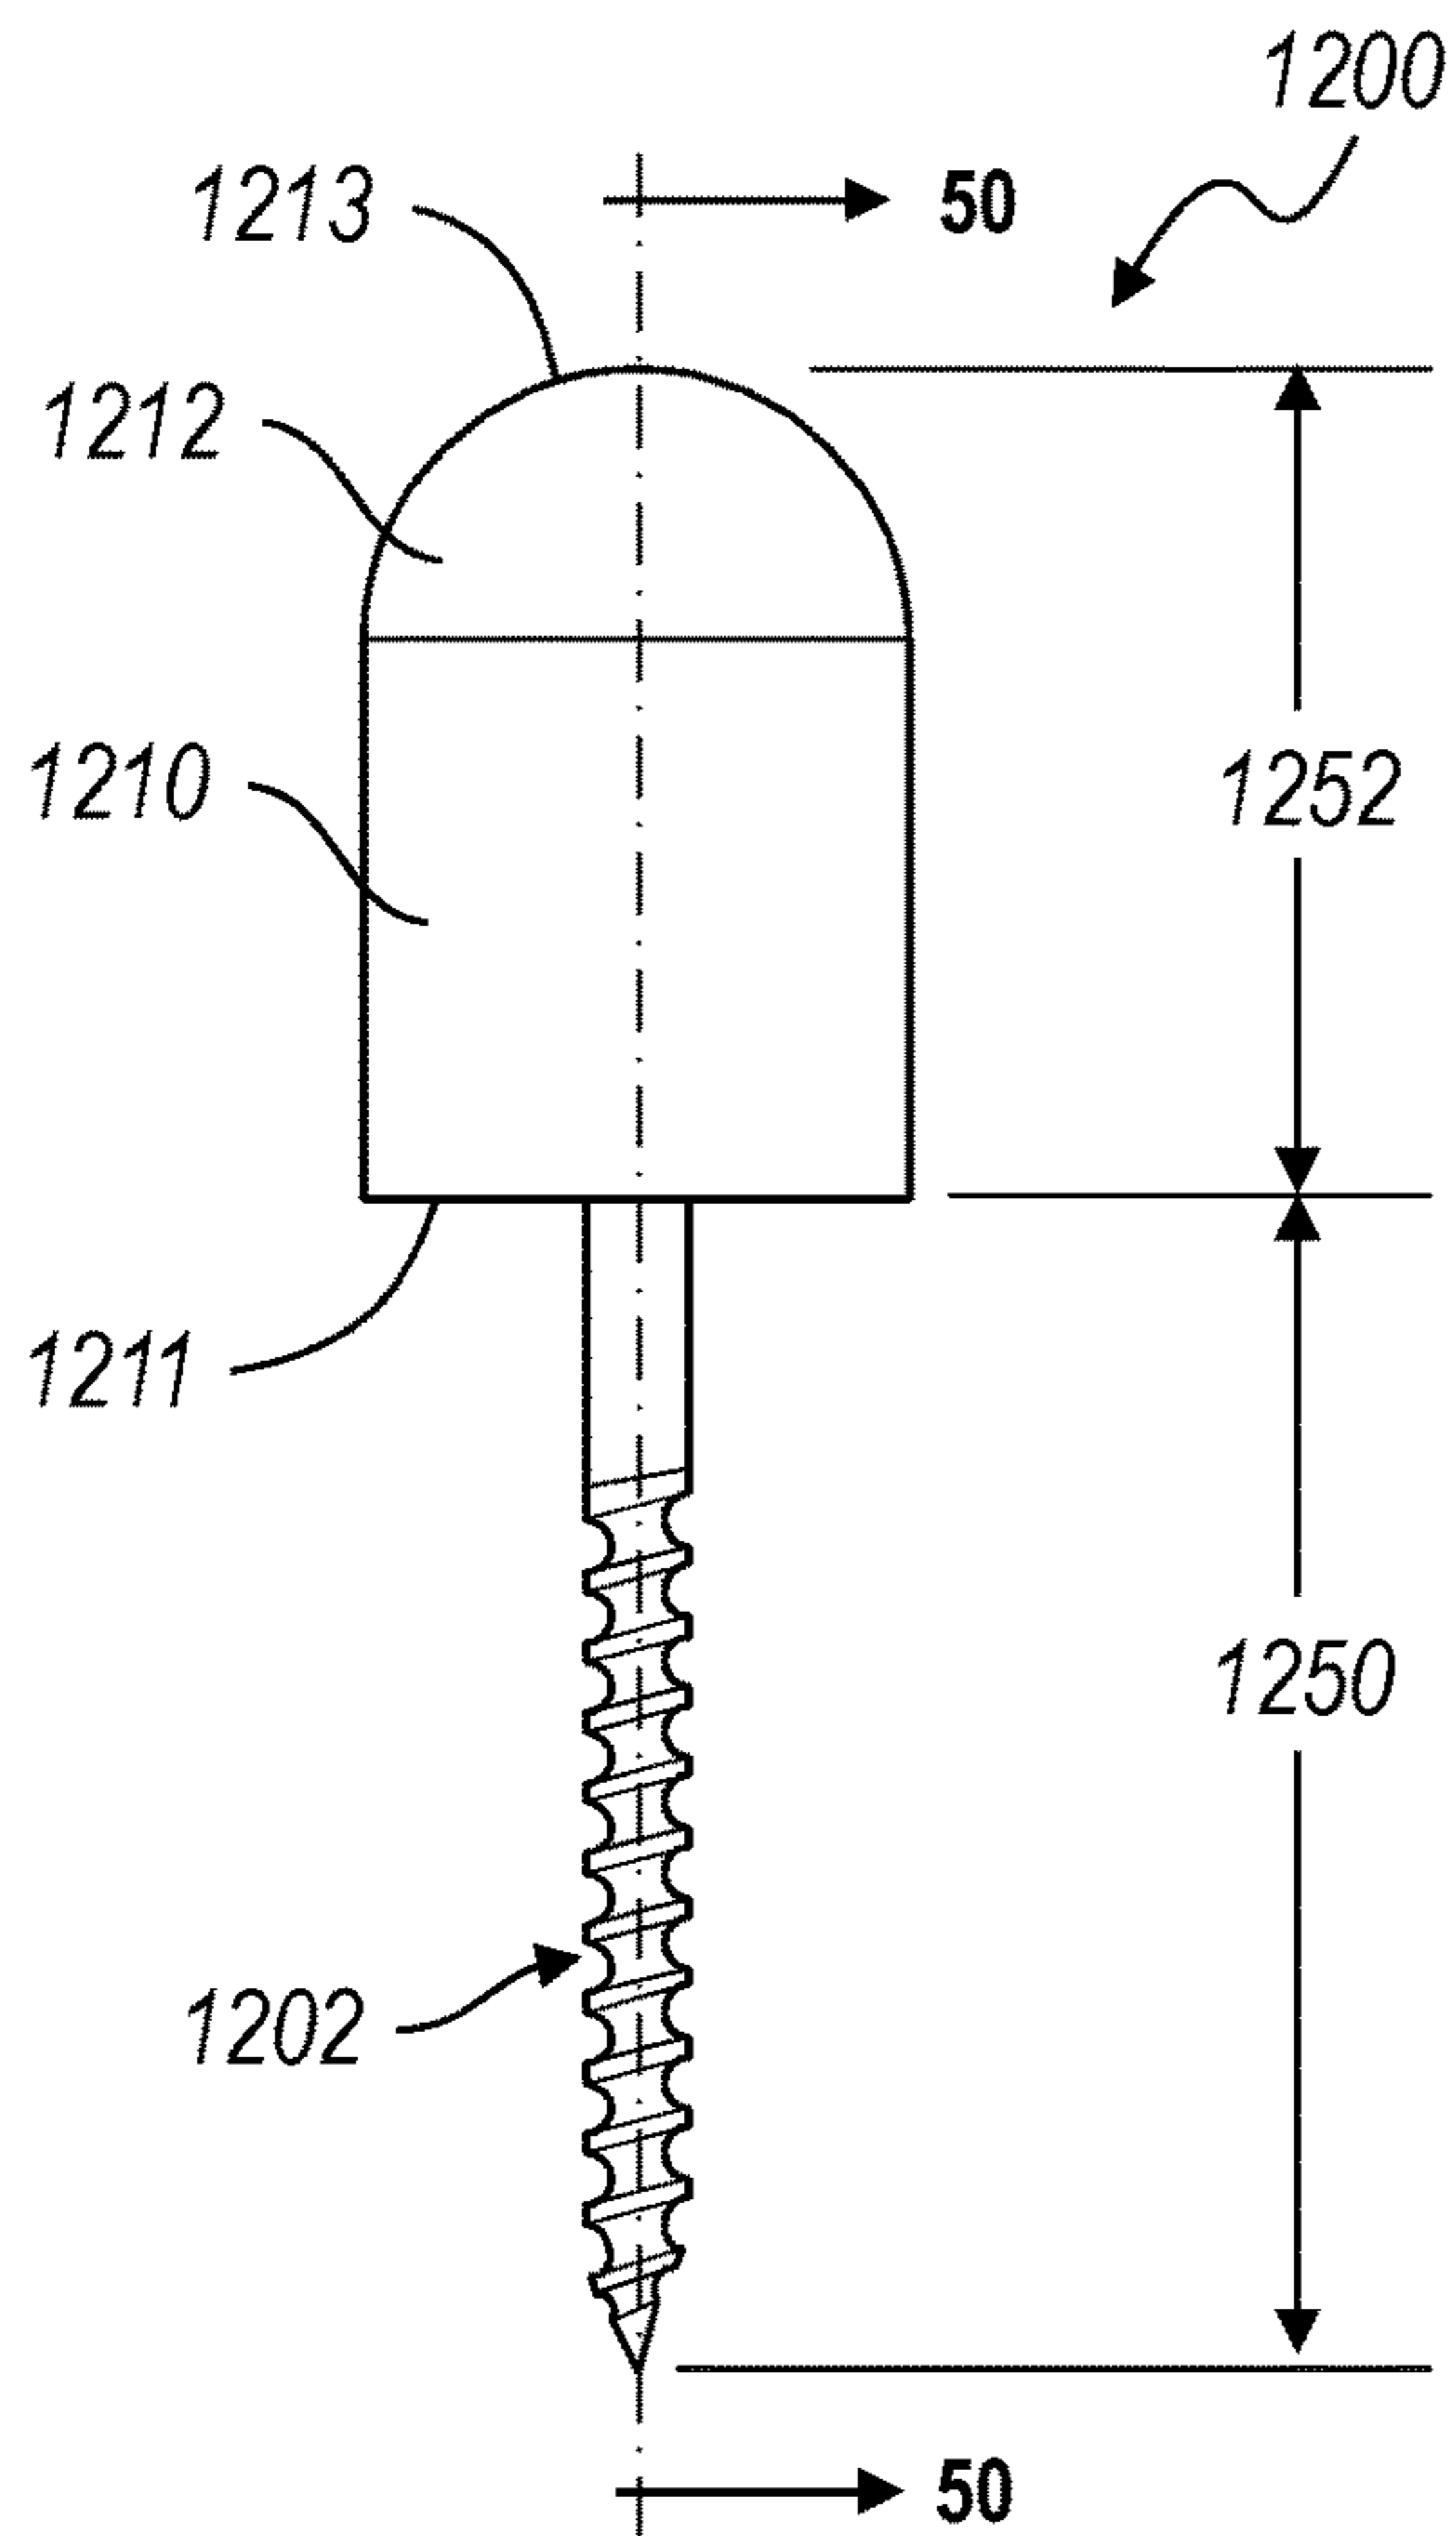


FIG. 49

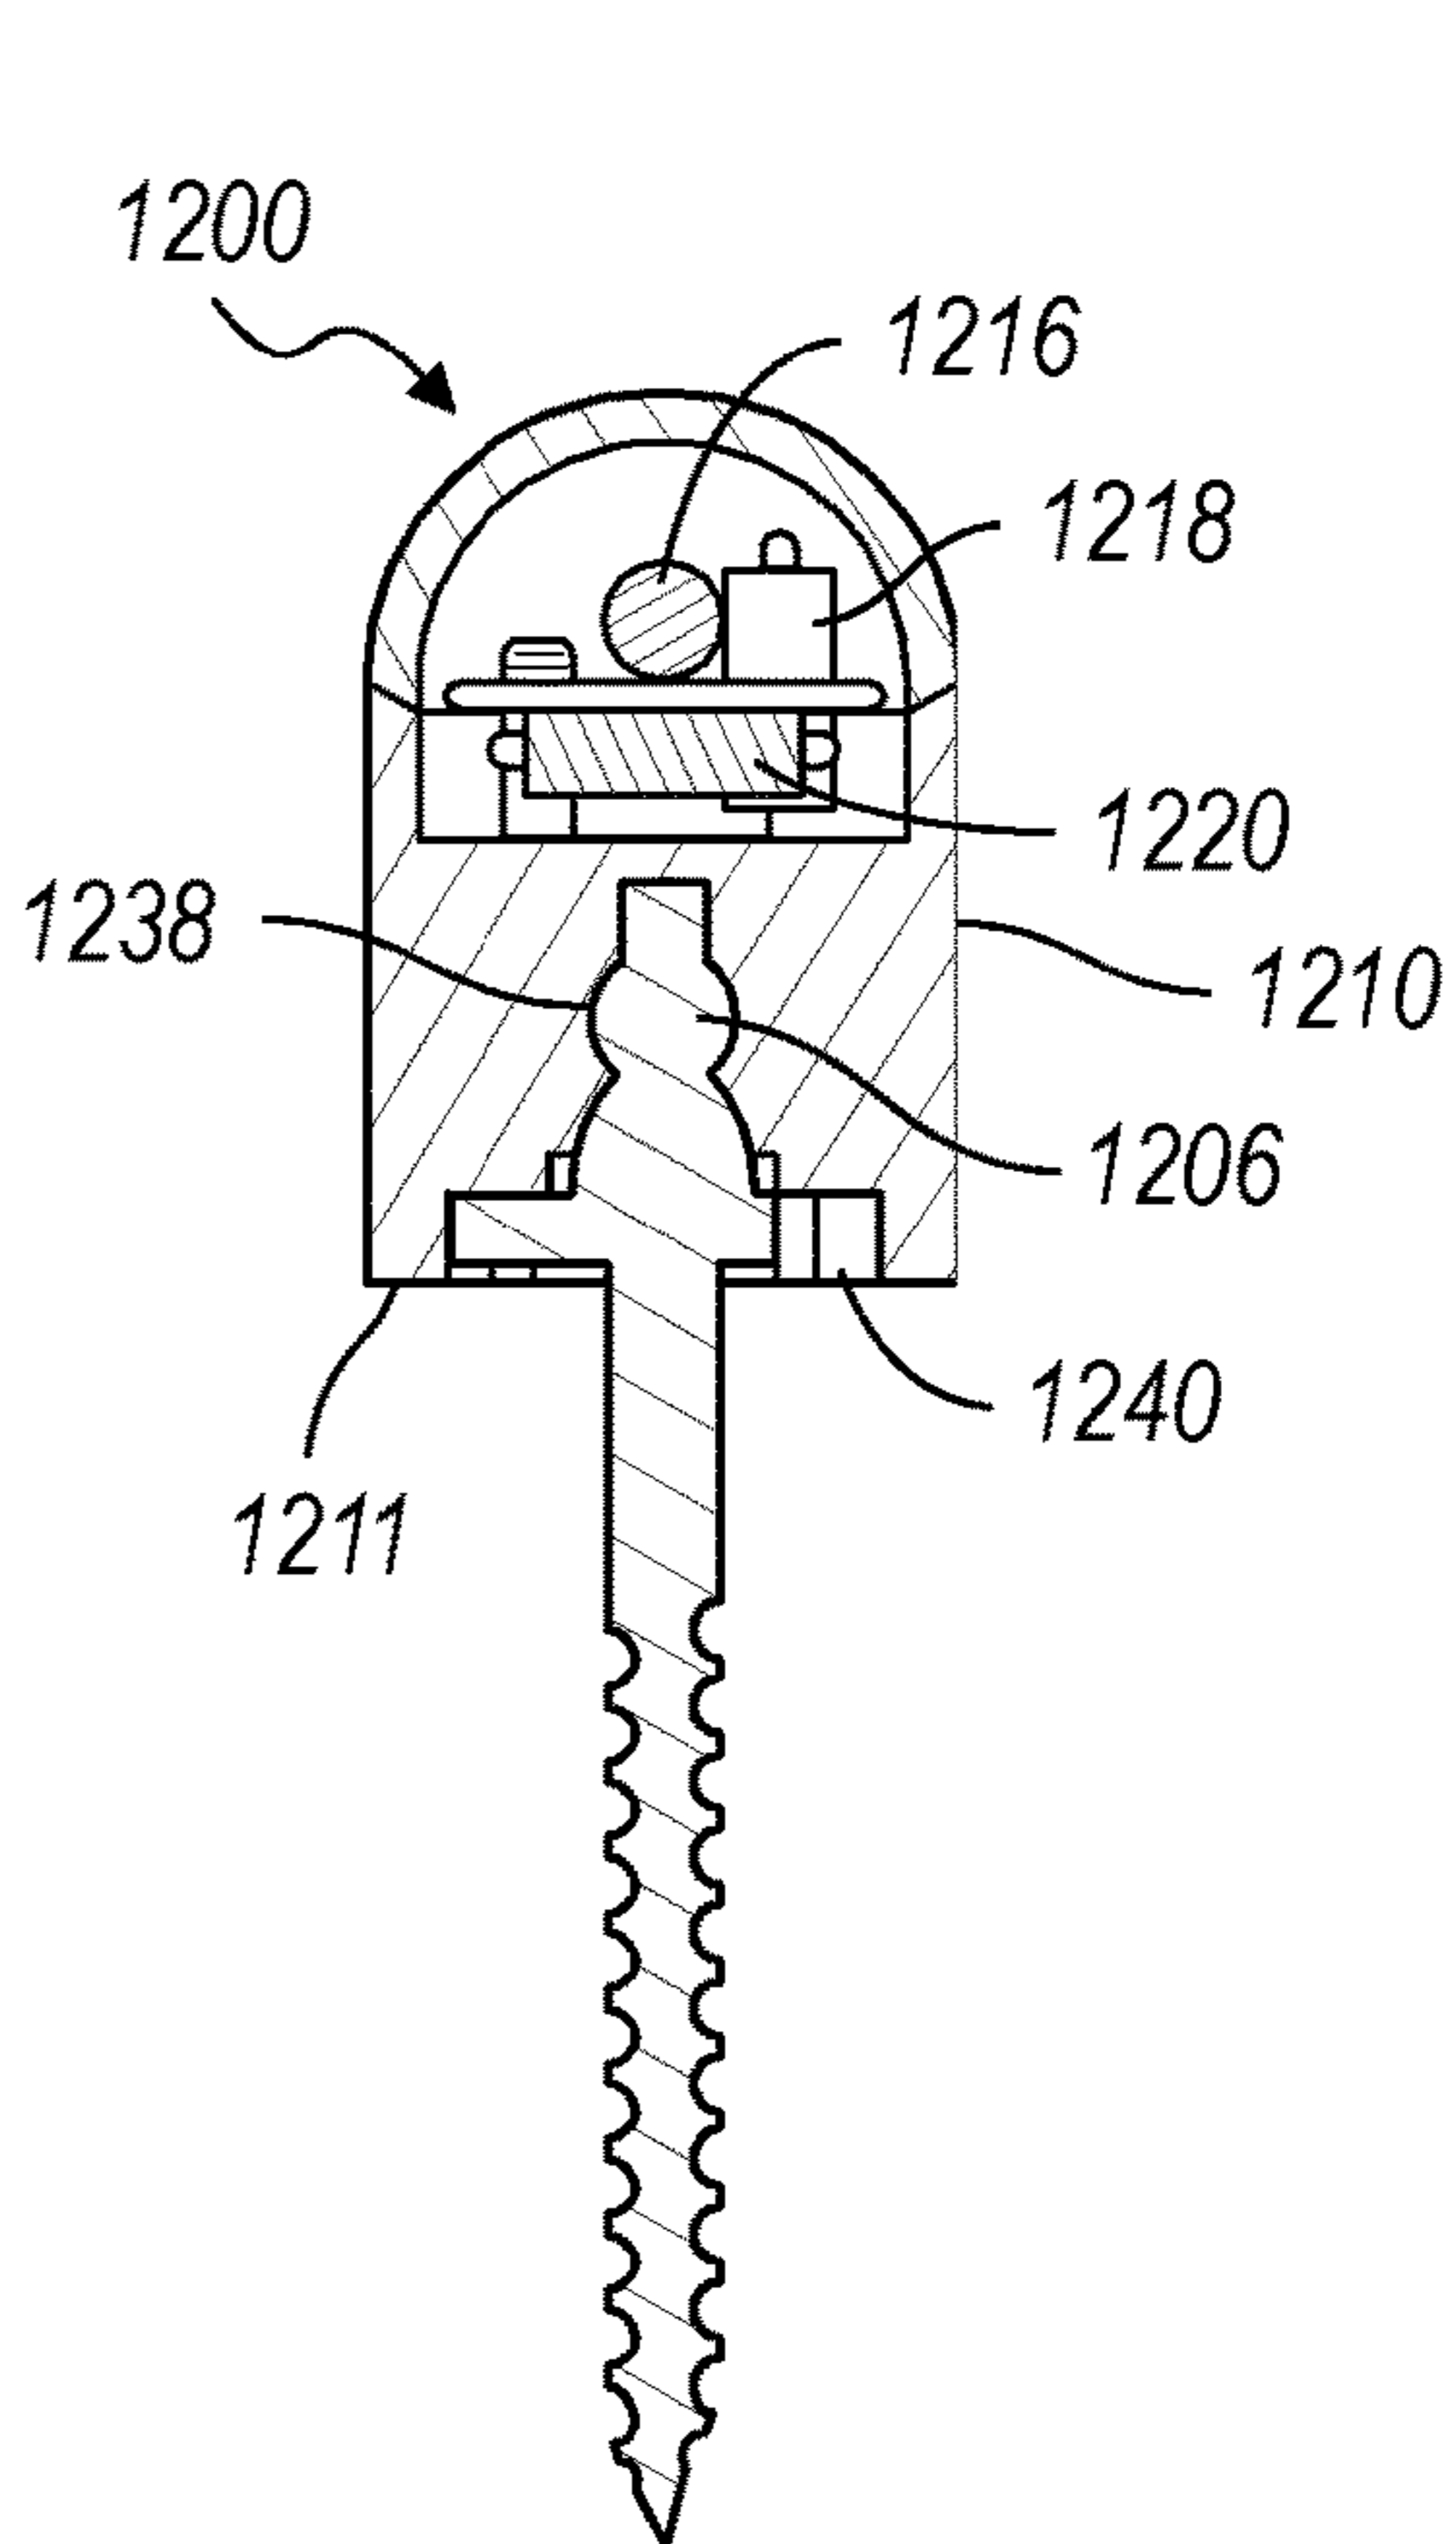


FIG. 50

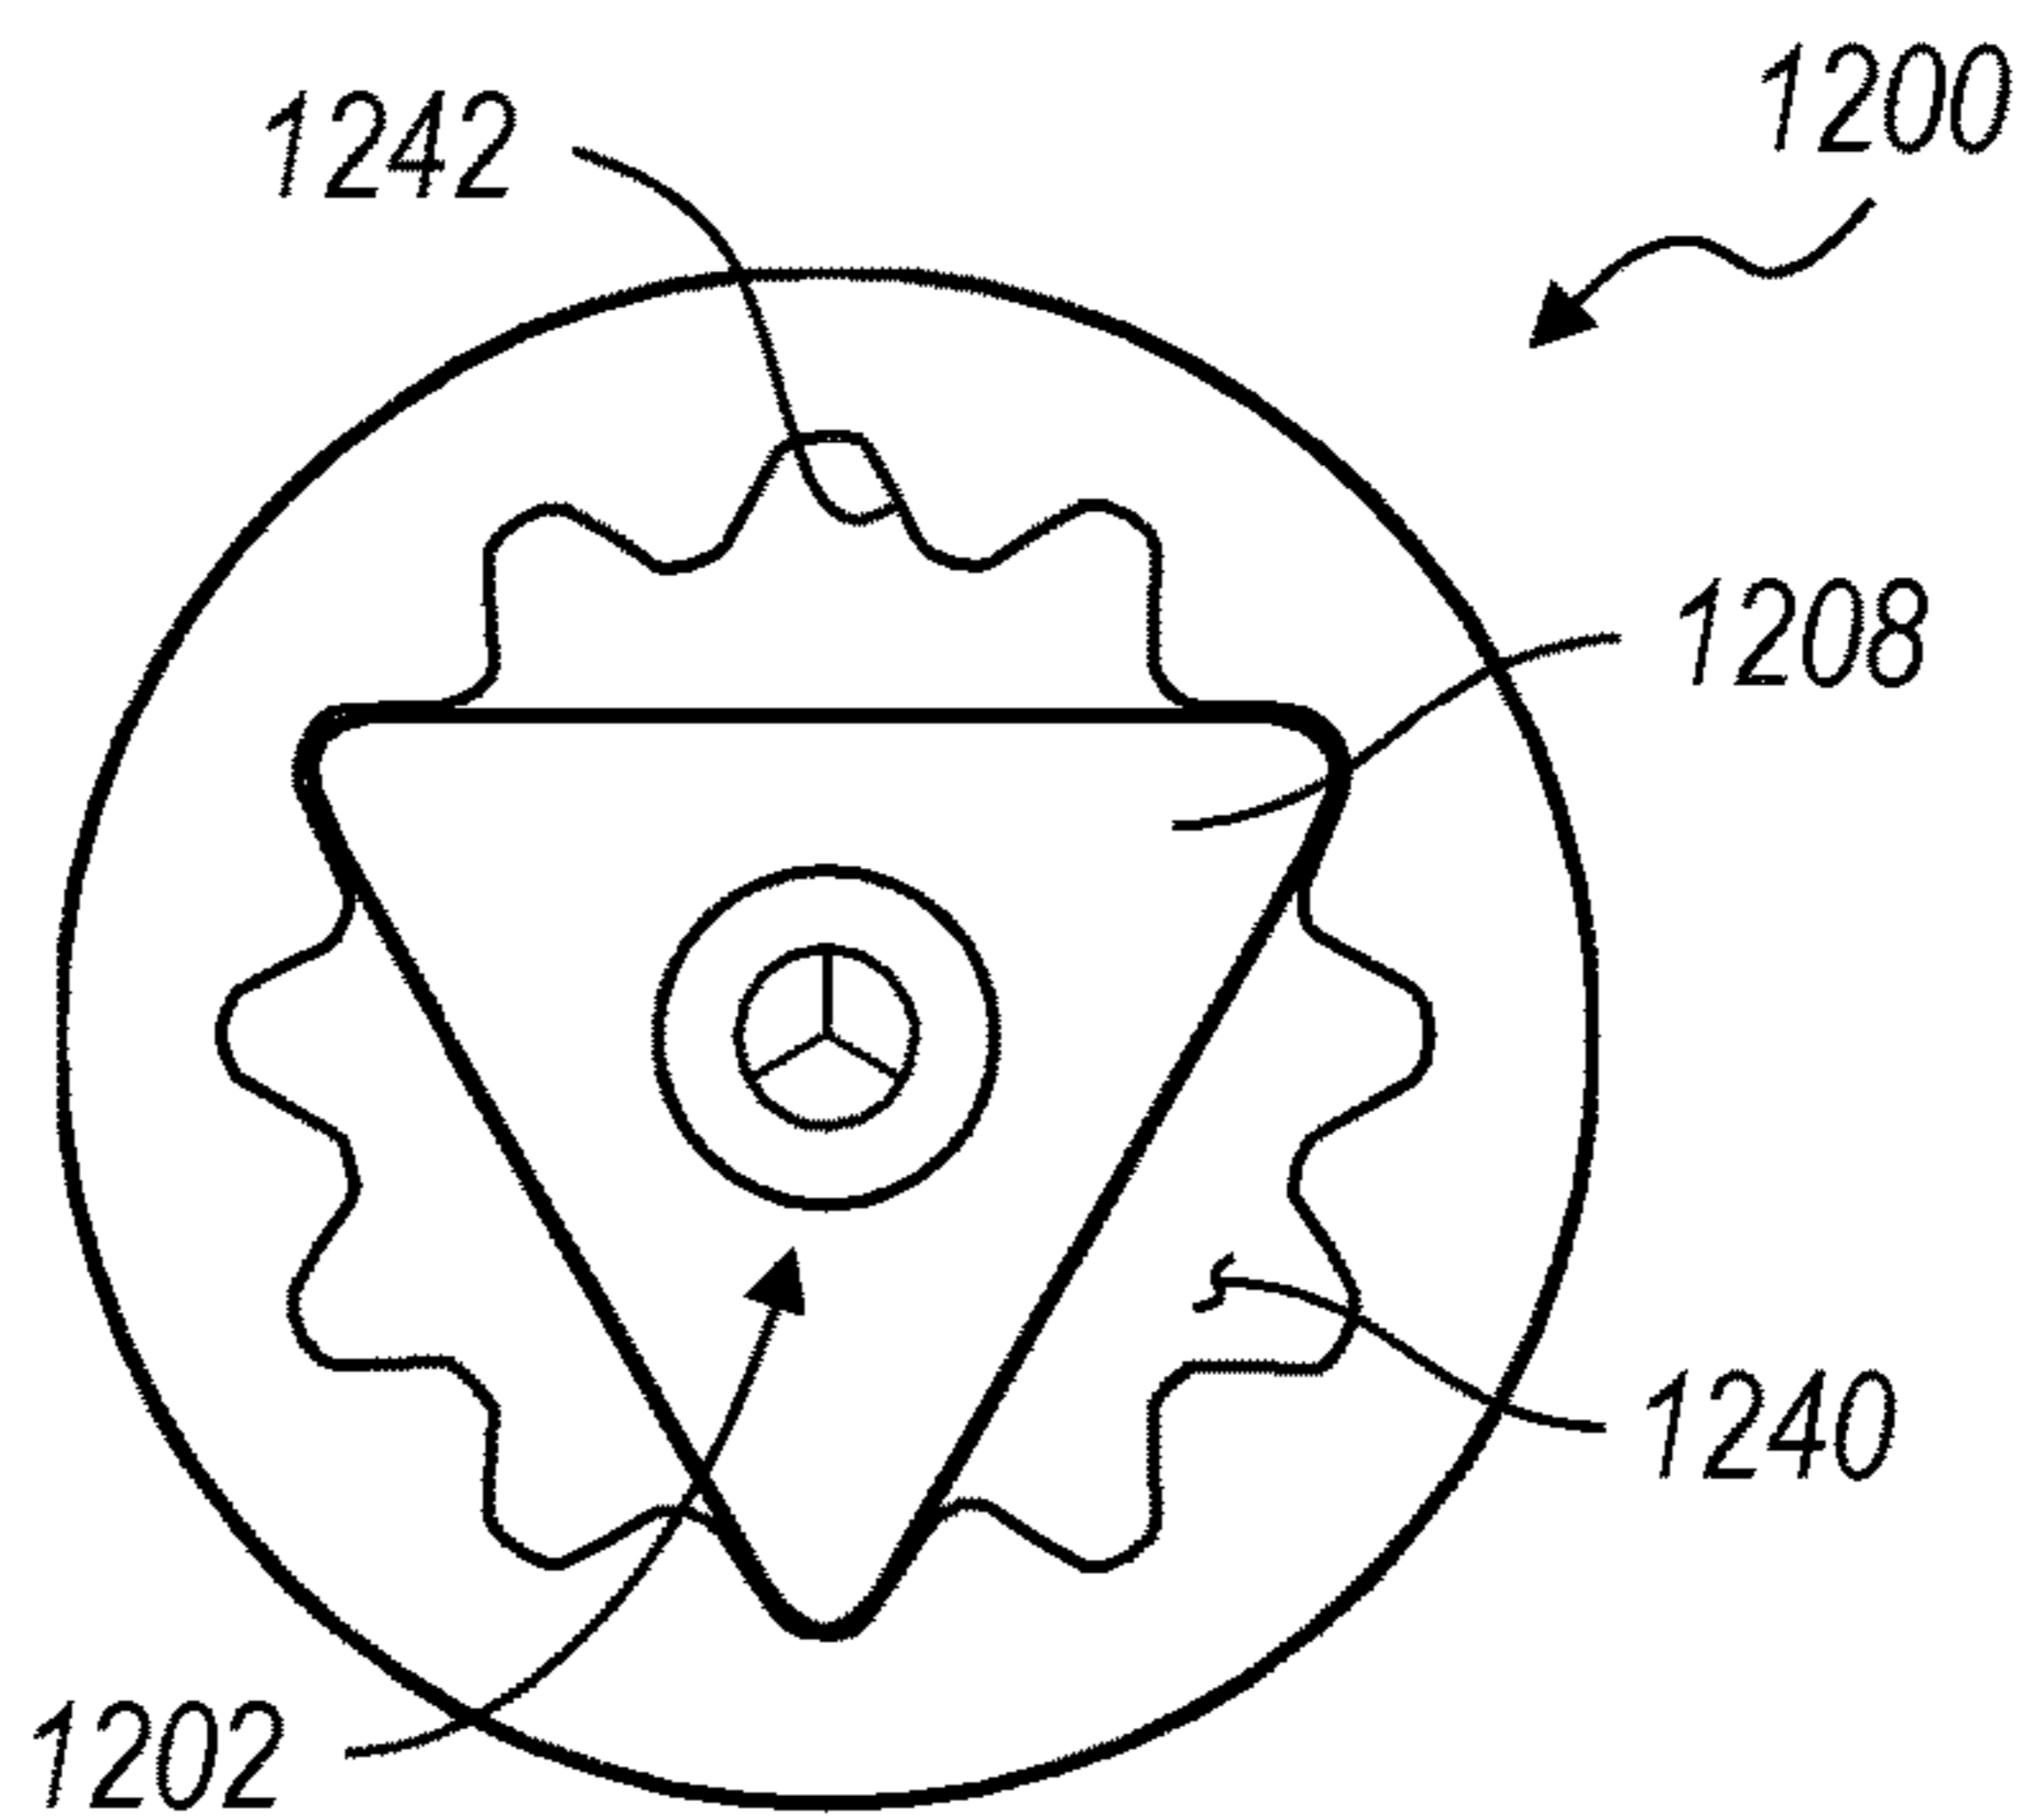


FIG. 51

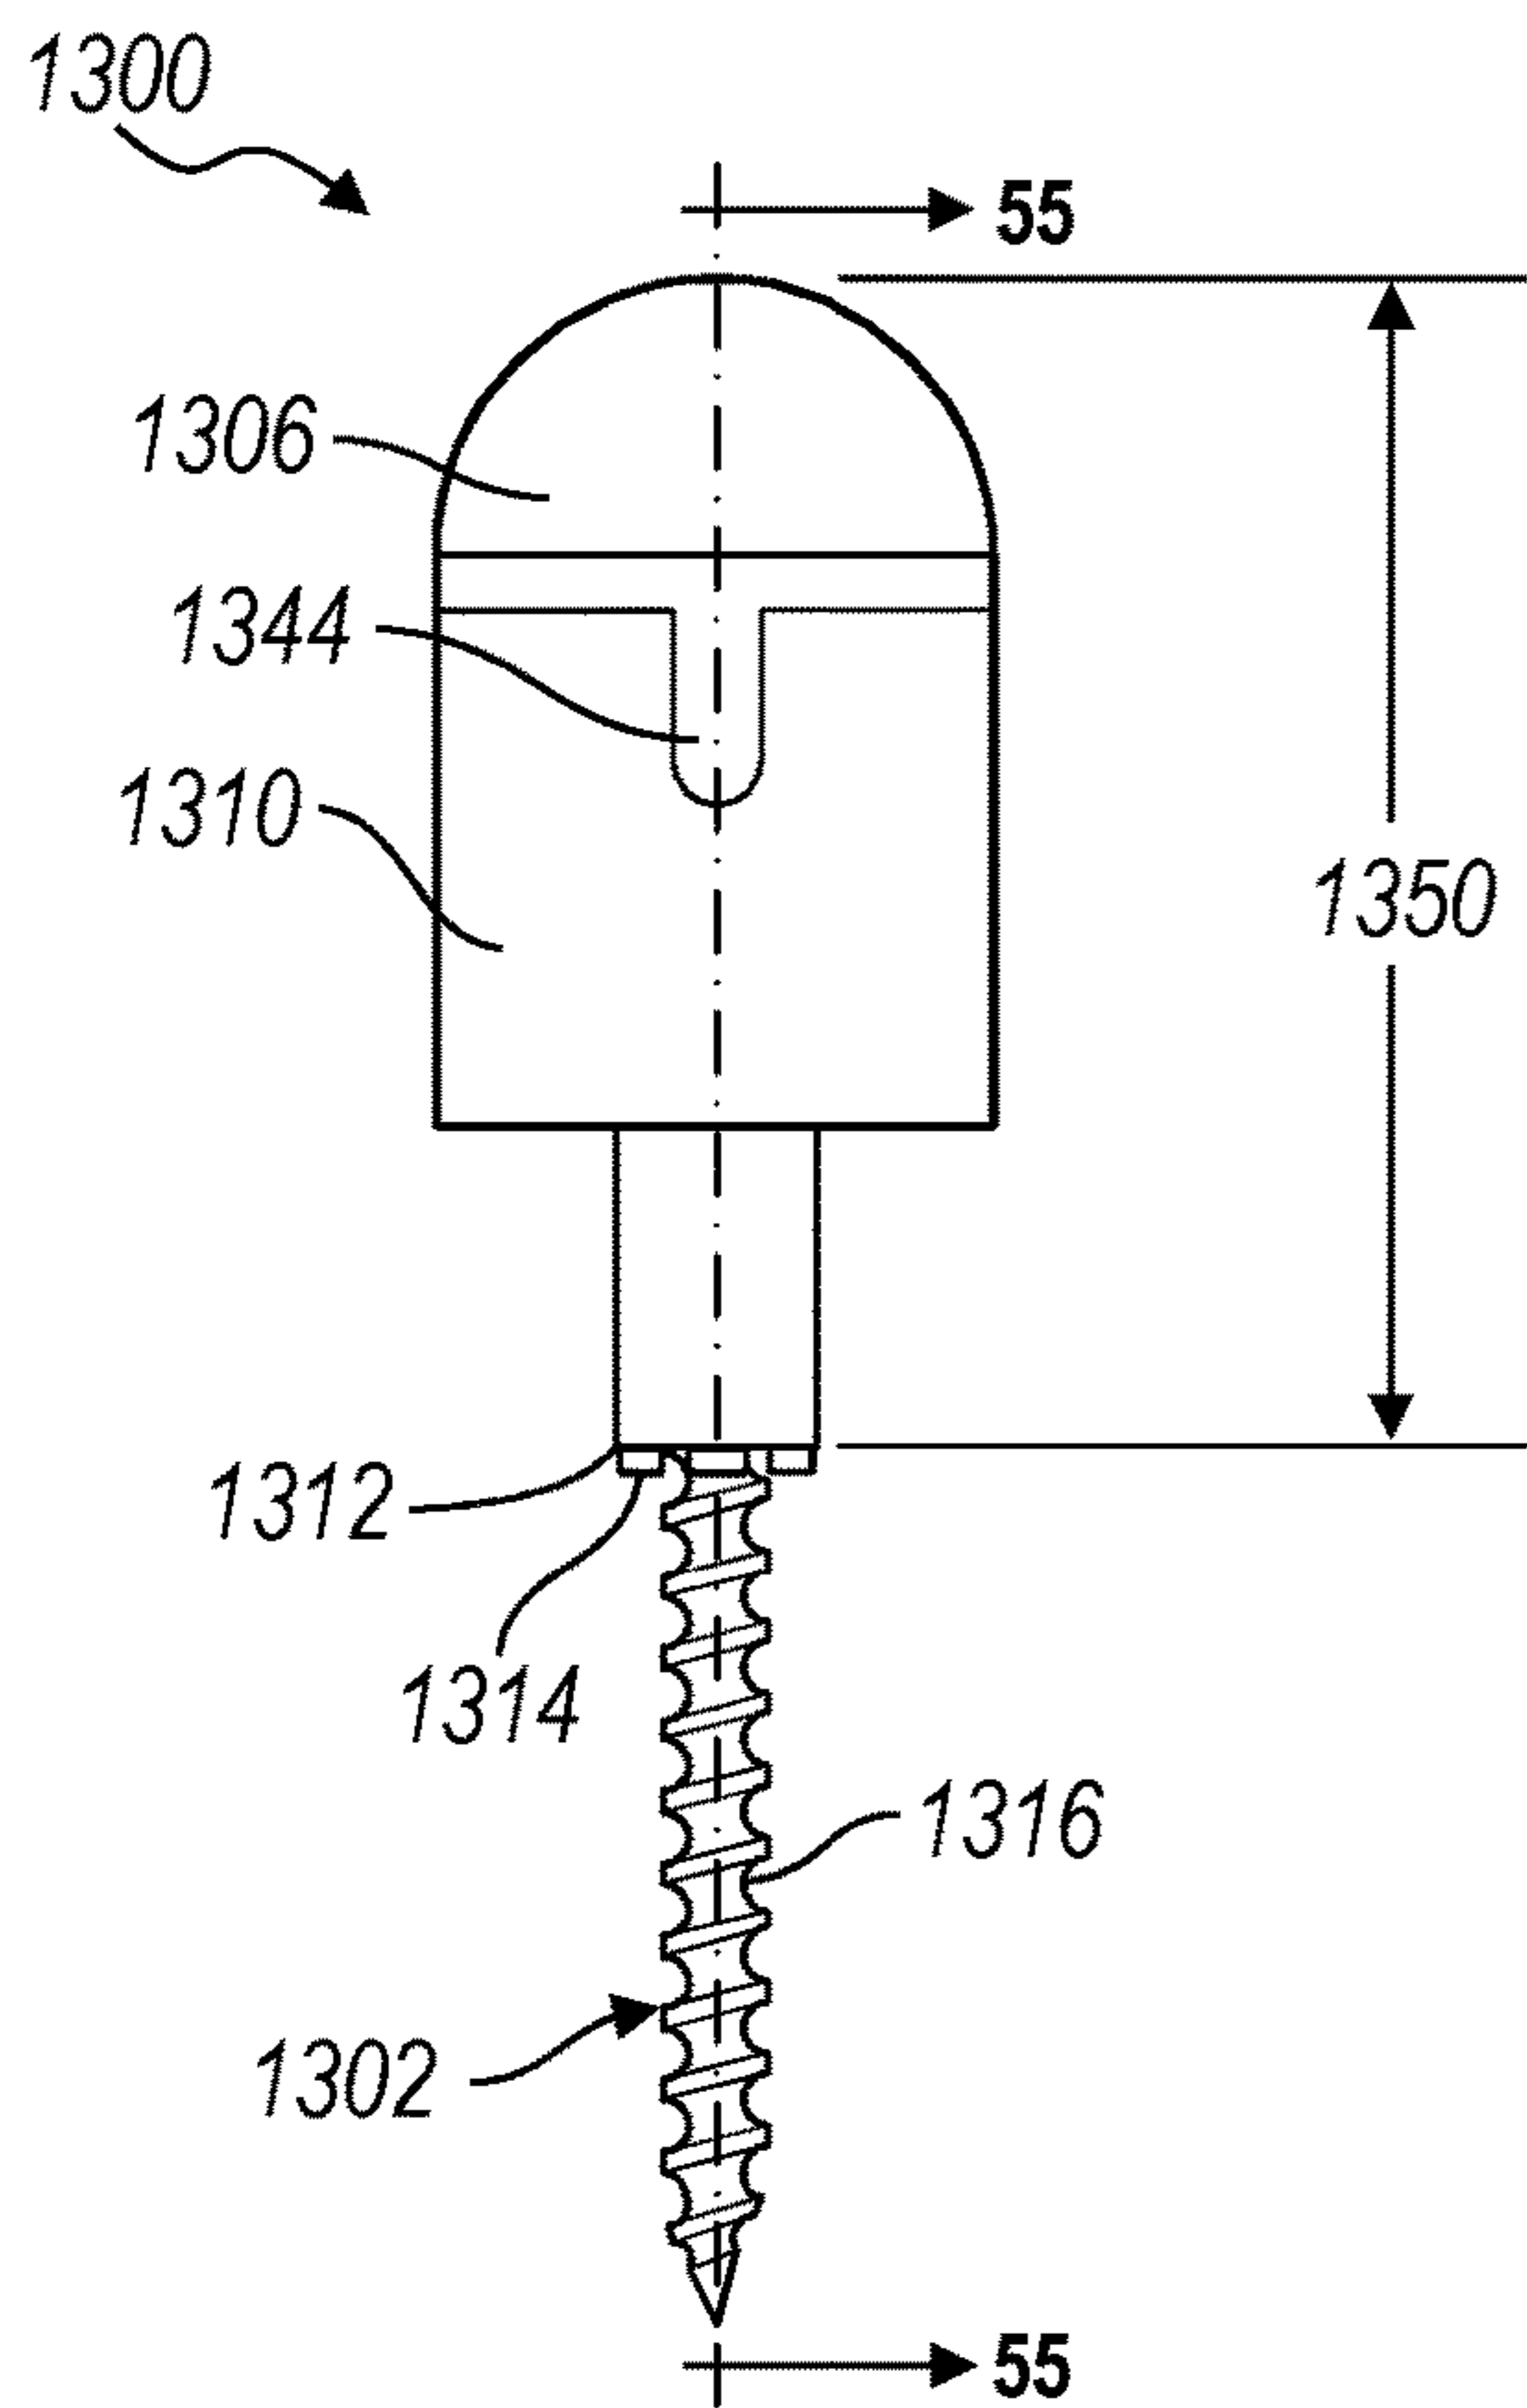


FIG. 54

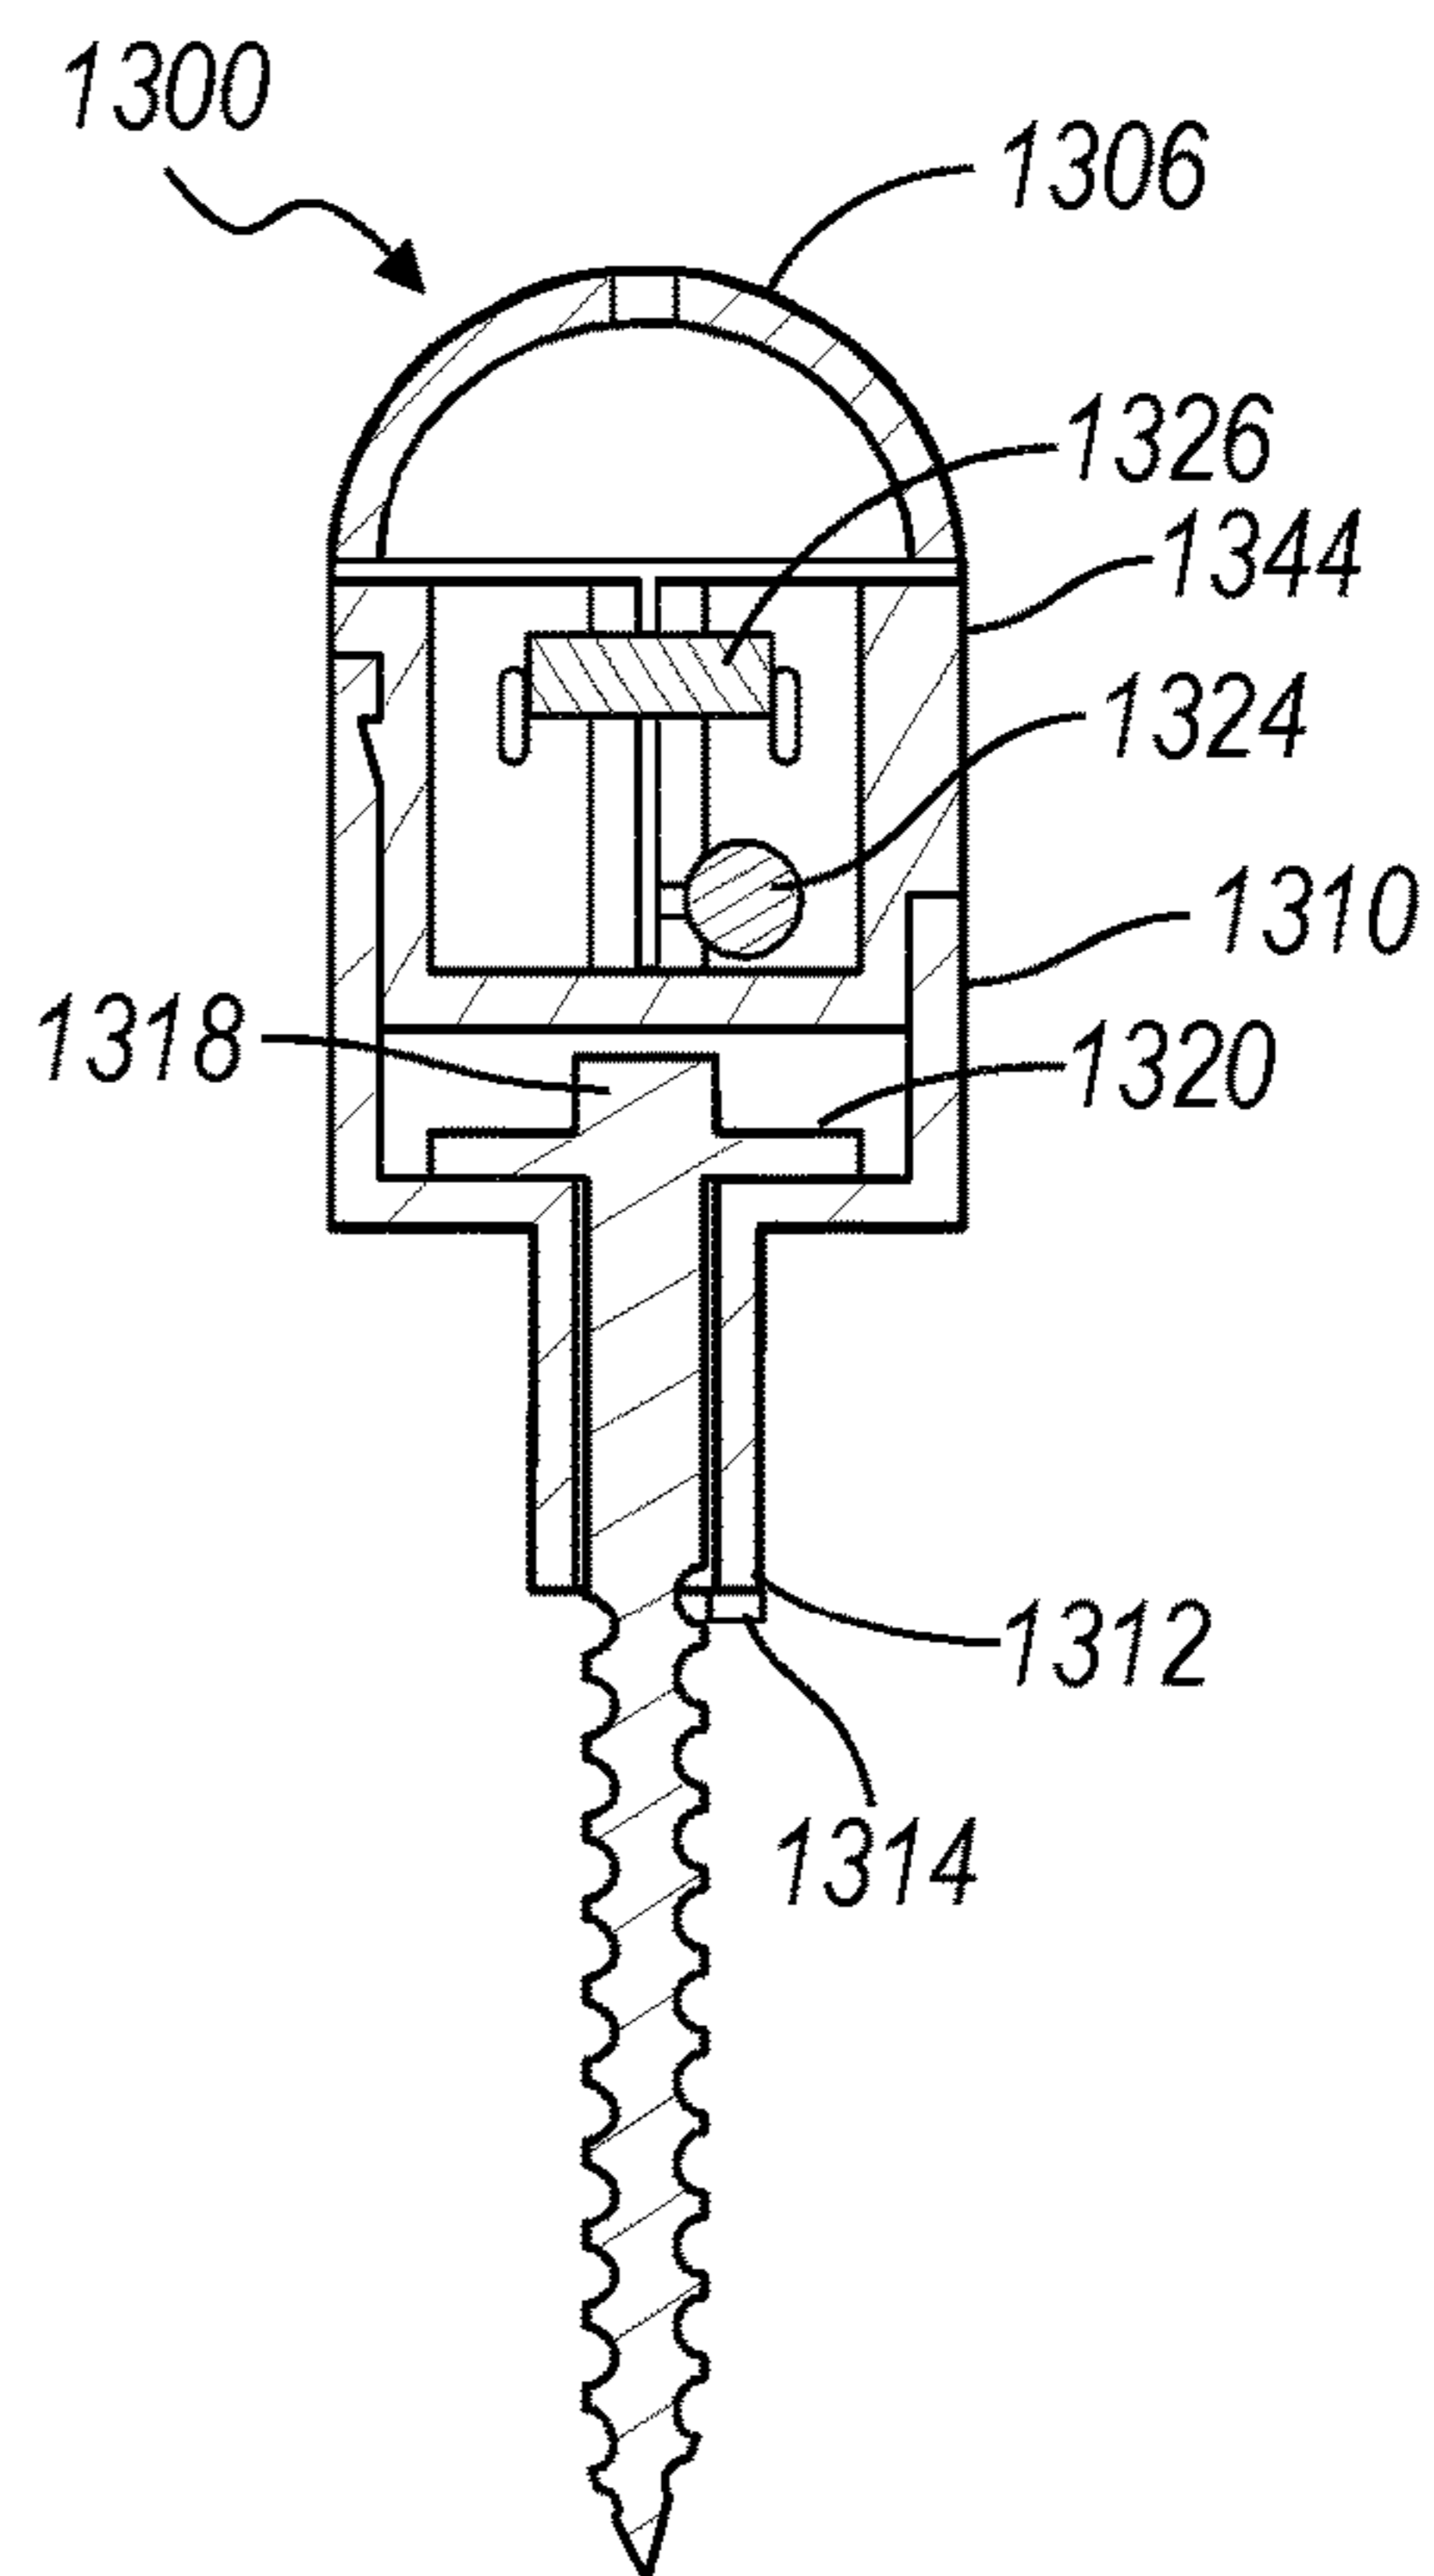


FIG. 55

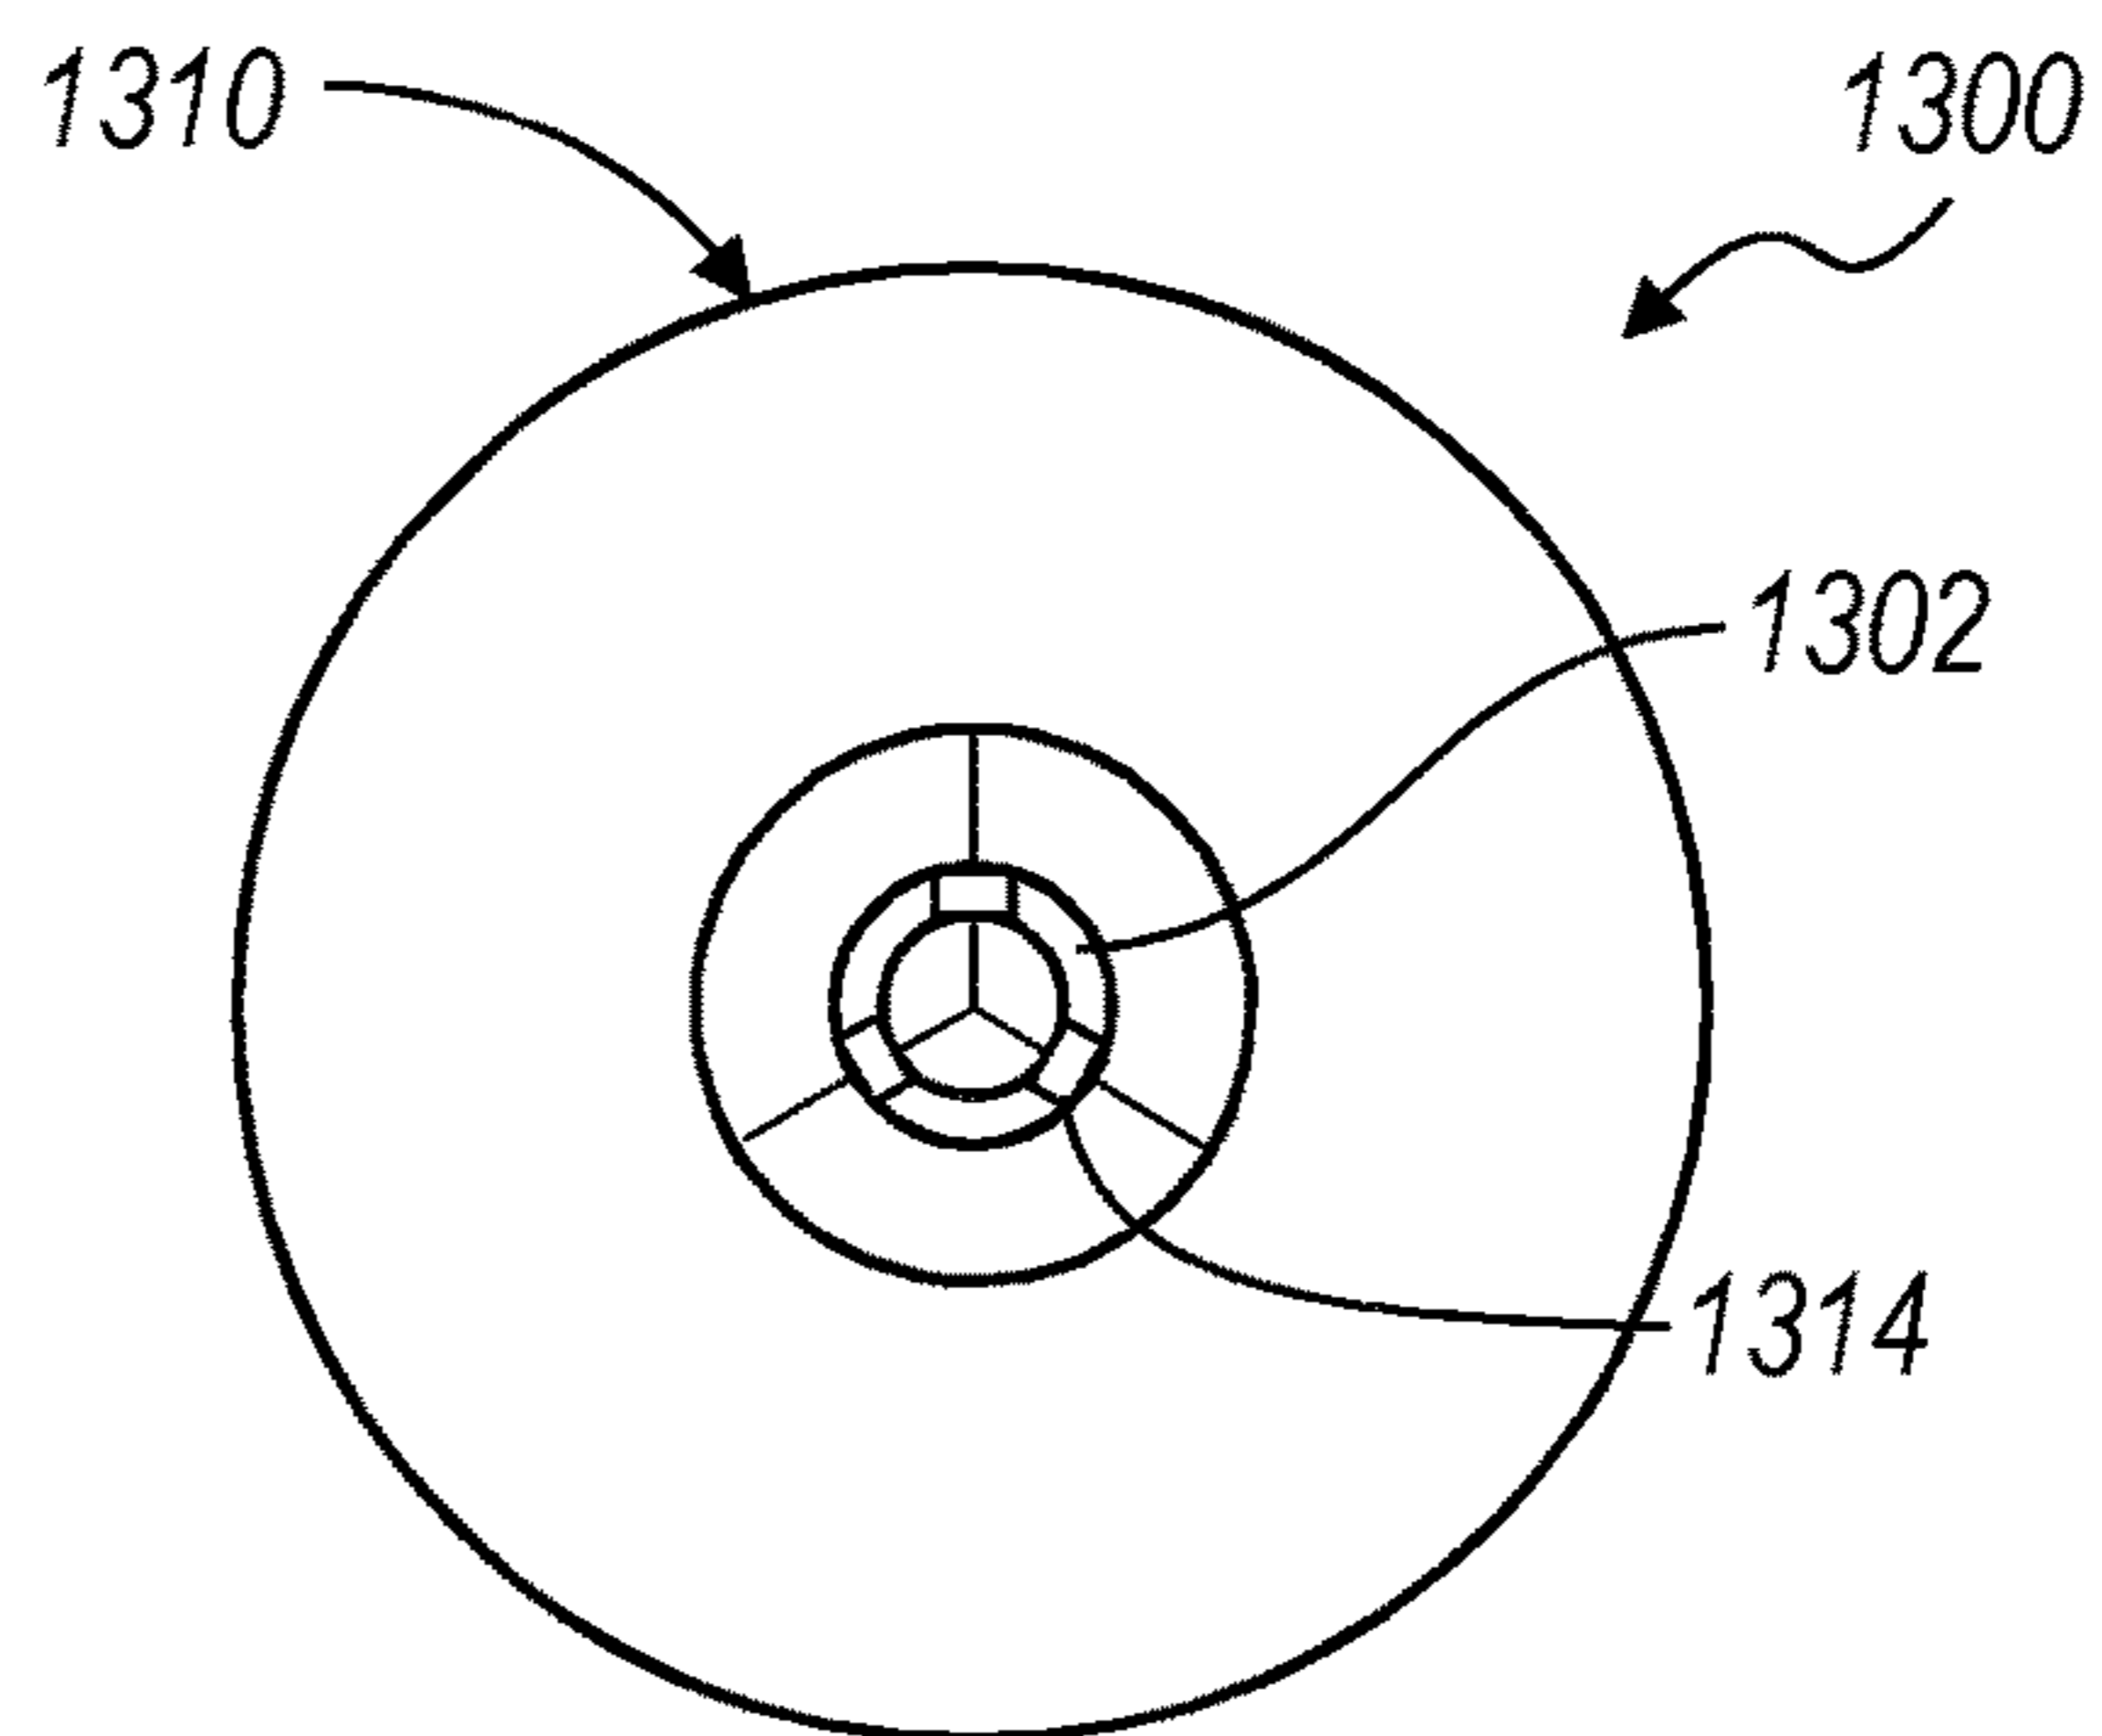


FIG. 56

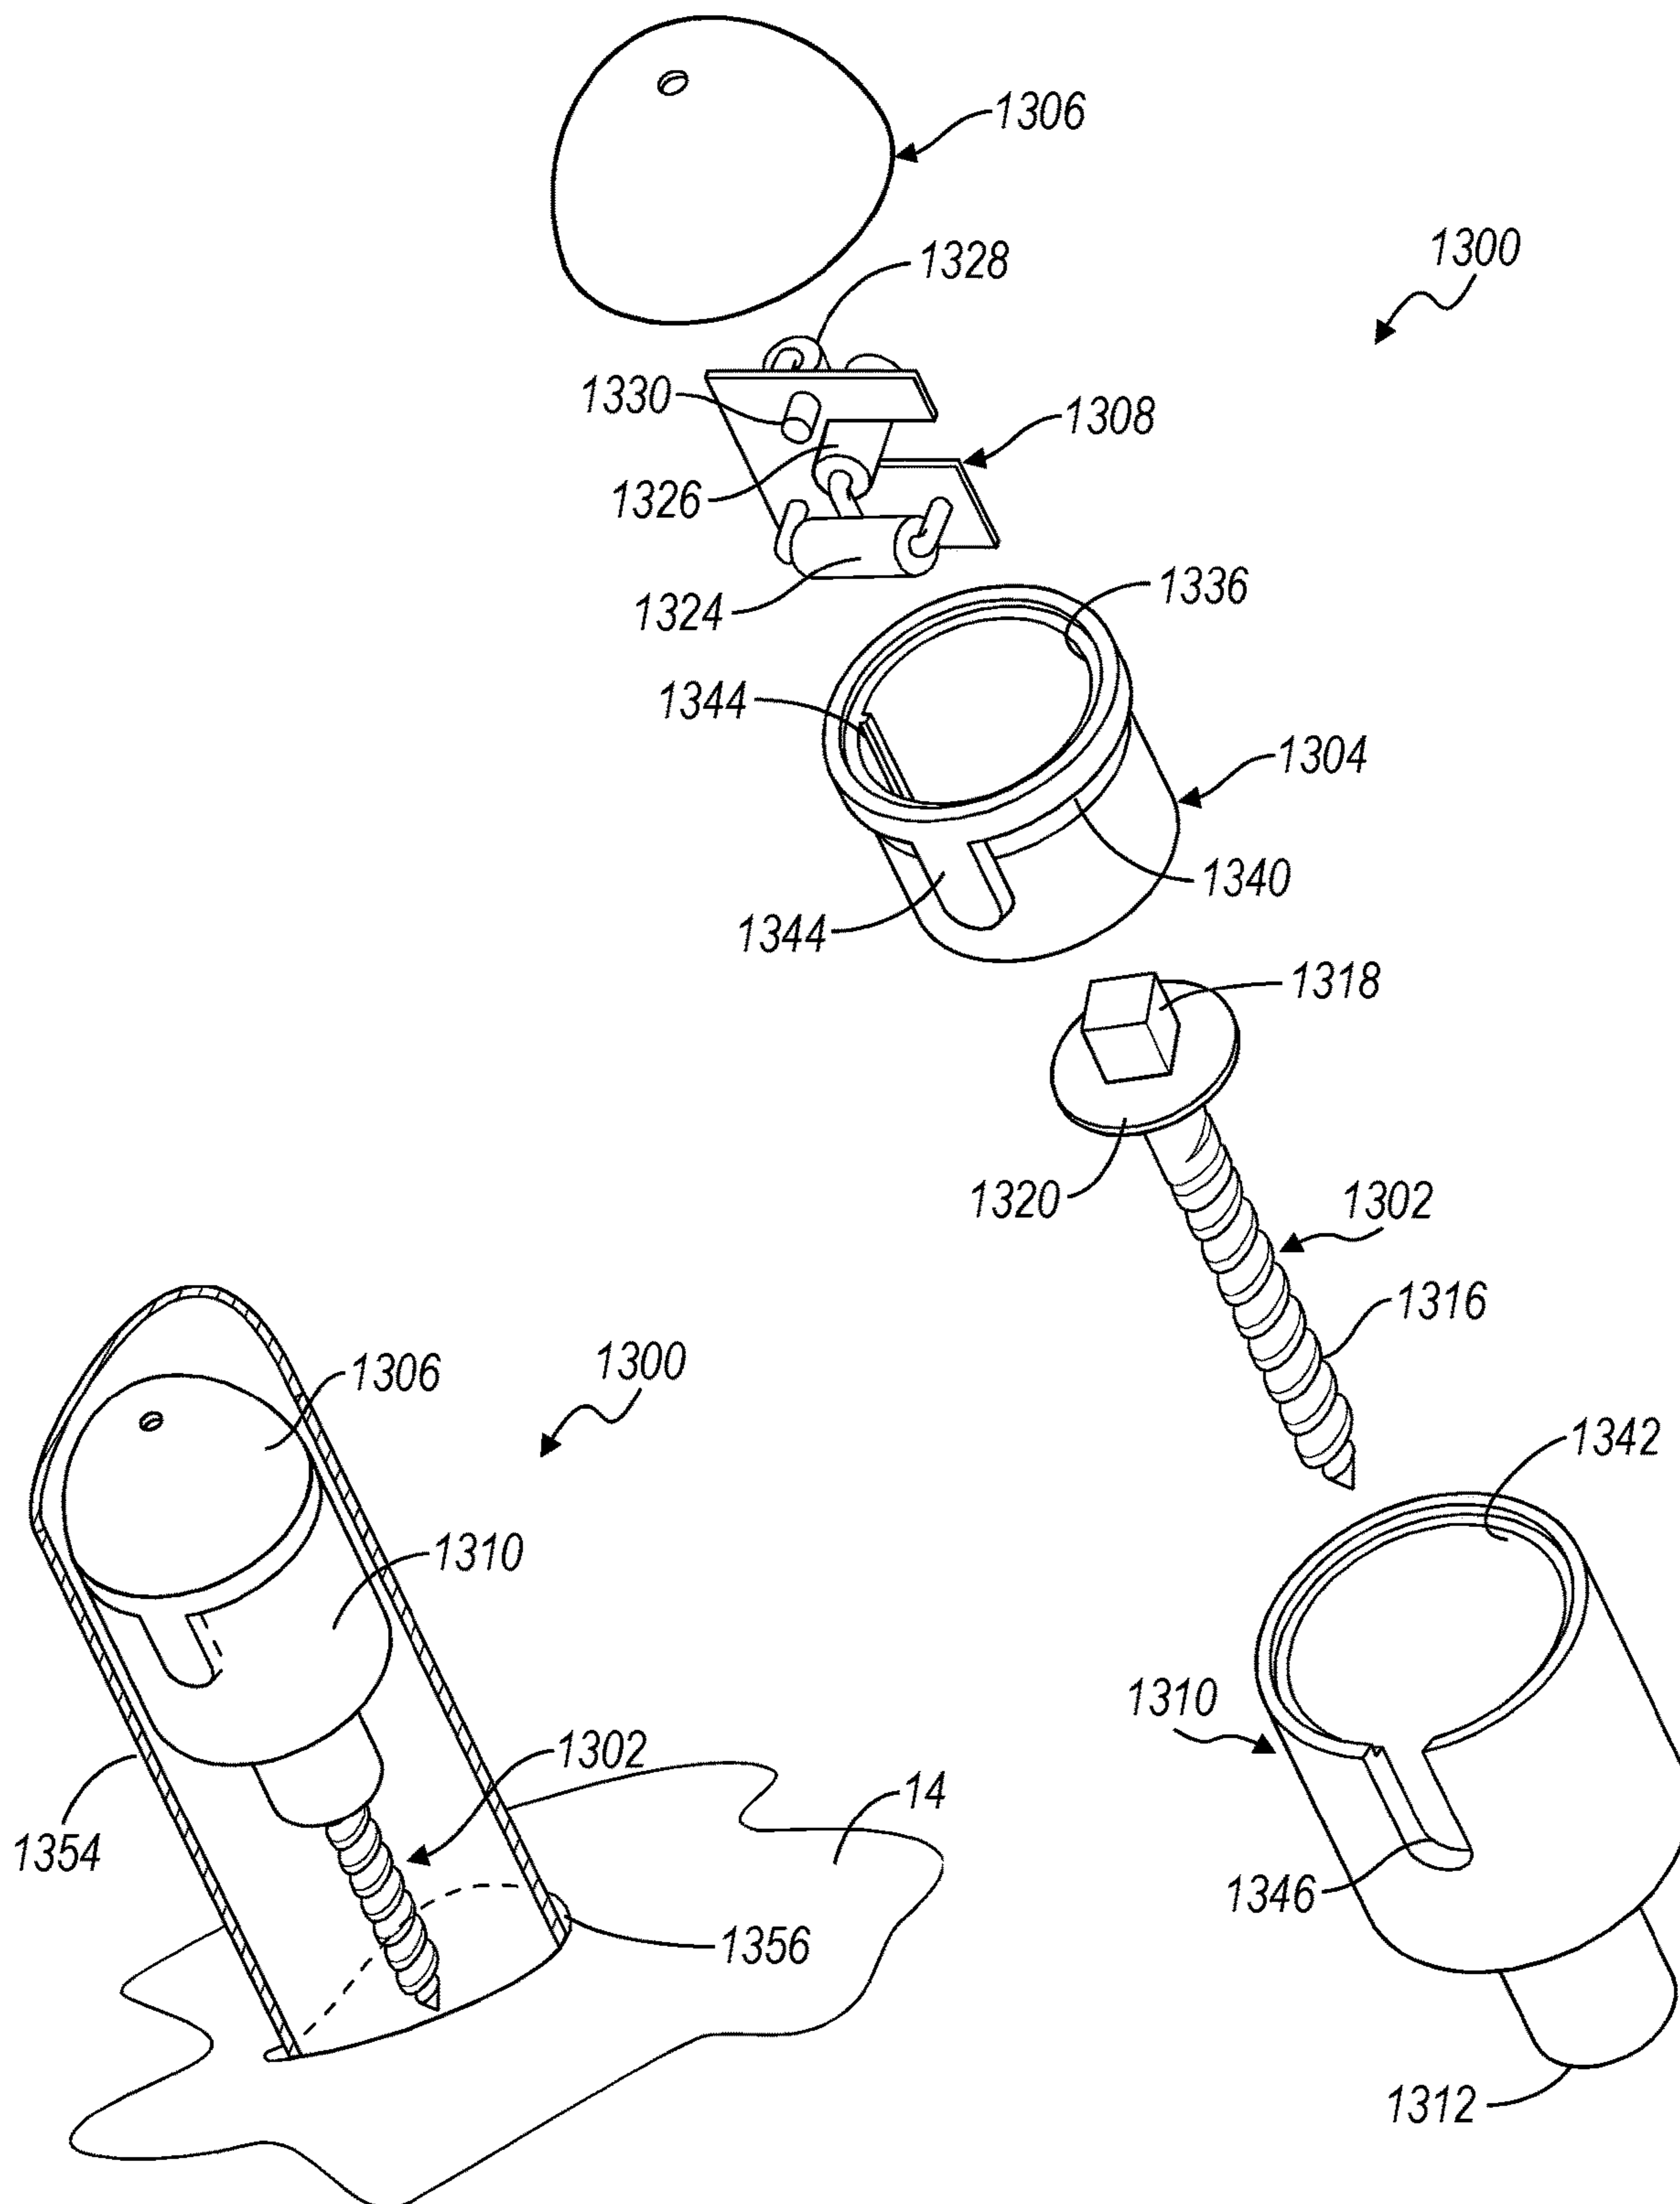


FIG. 58

FIG. 57

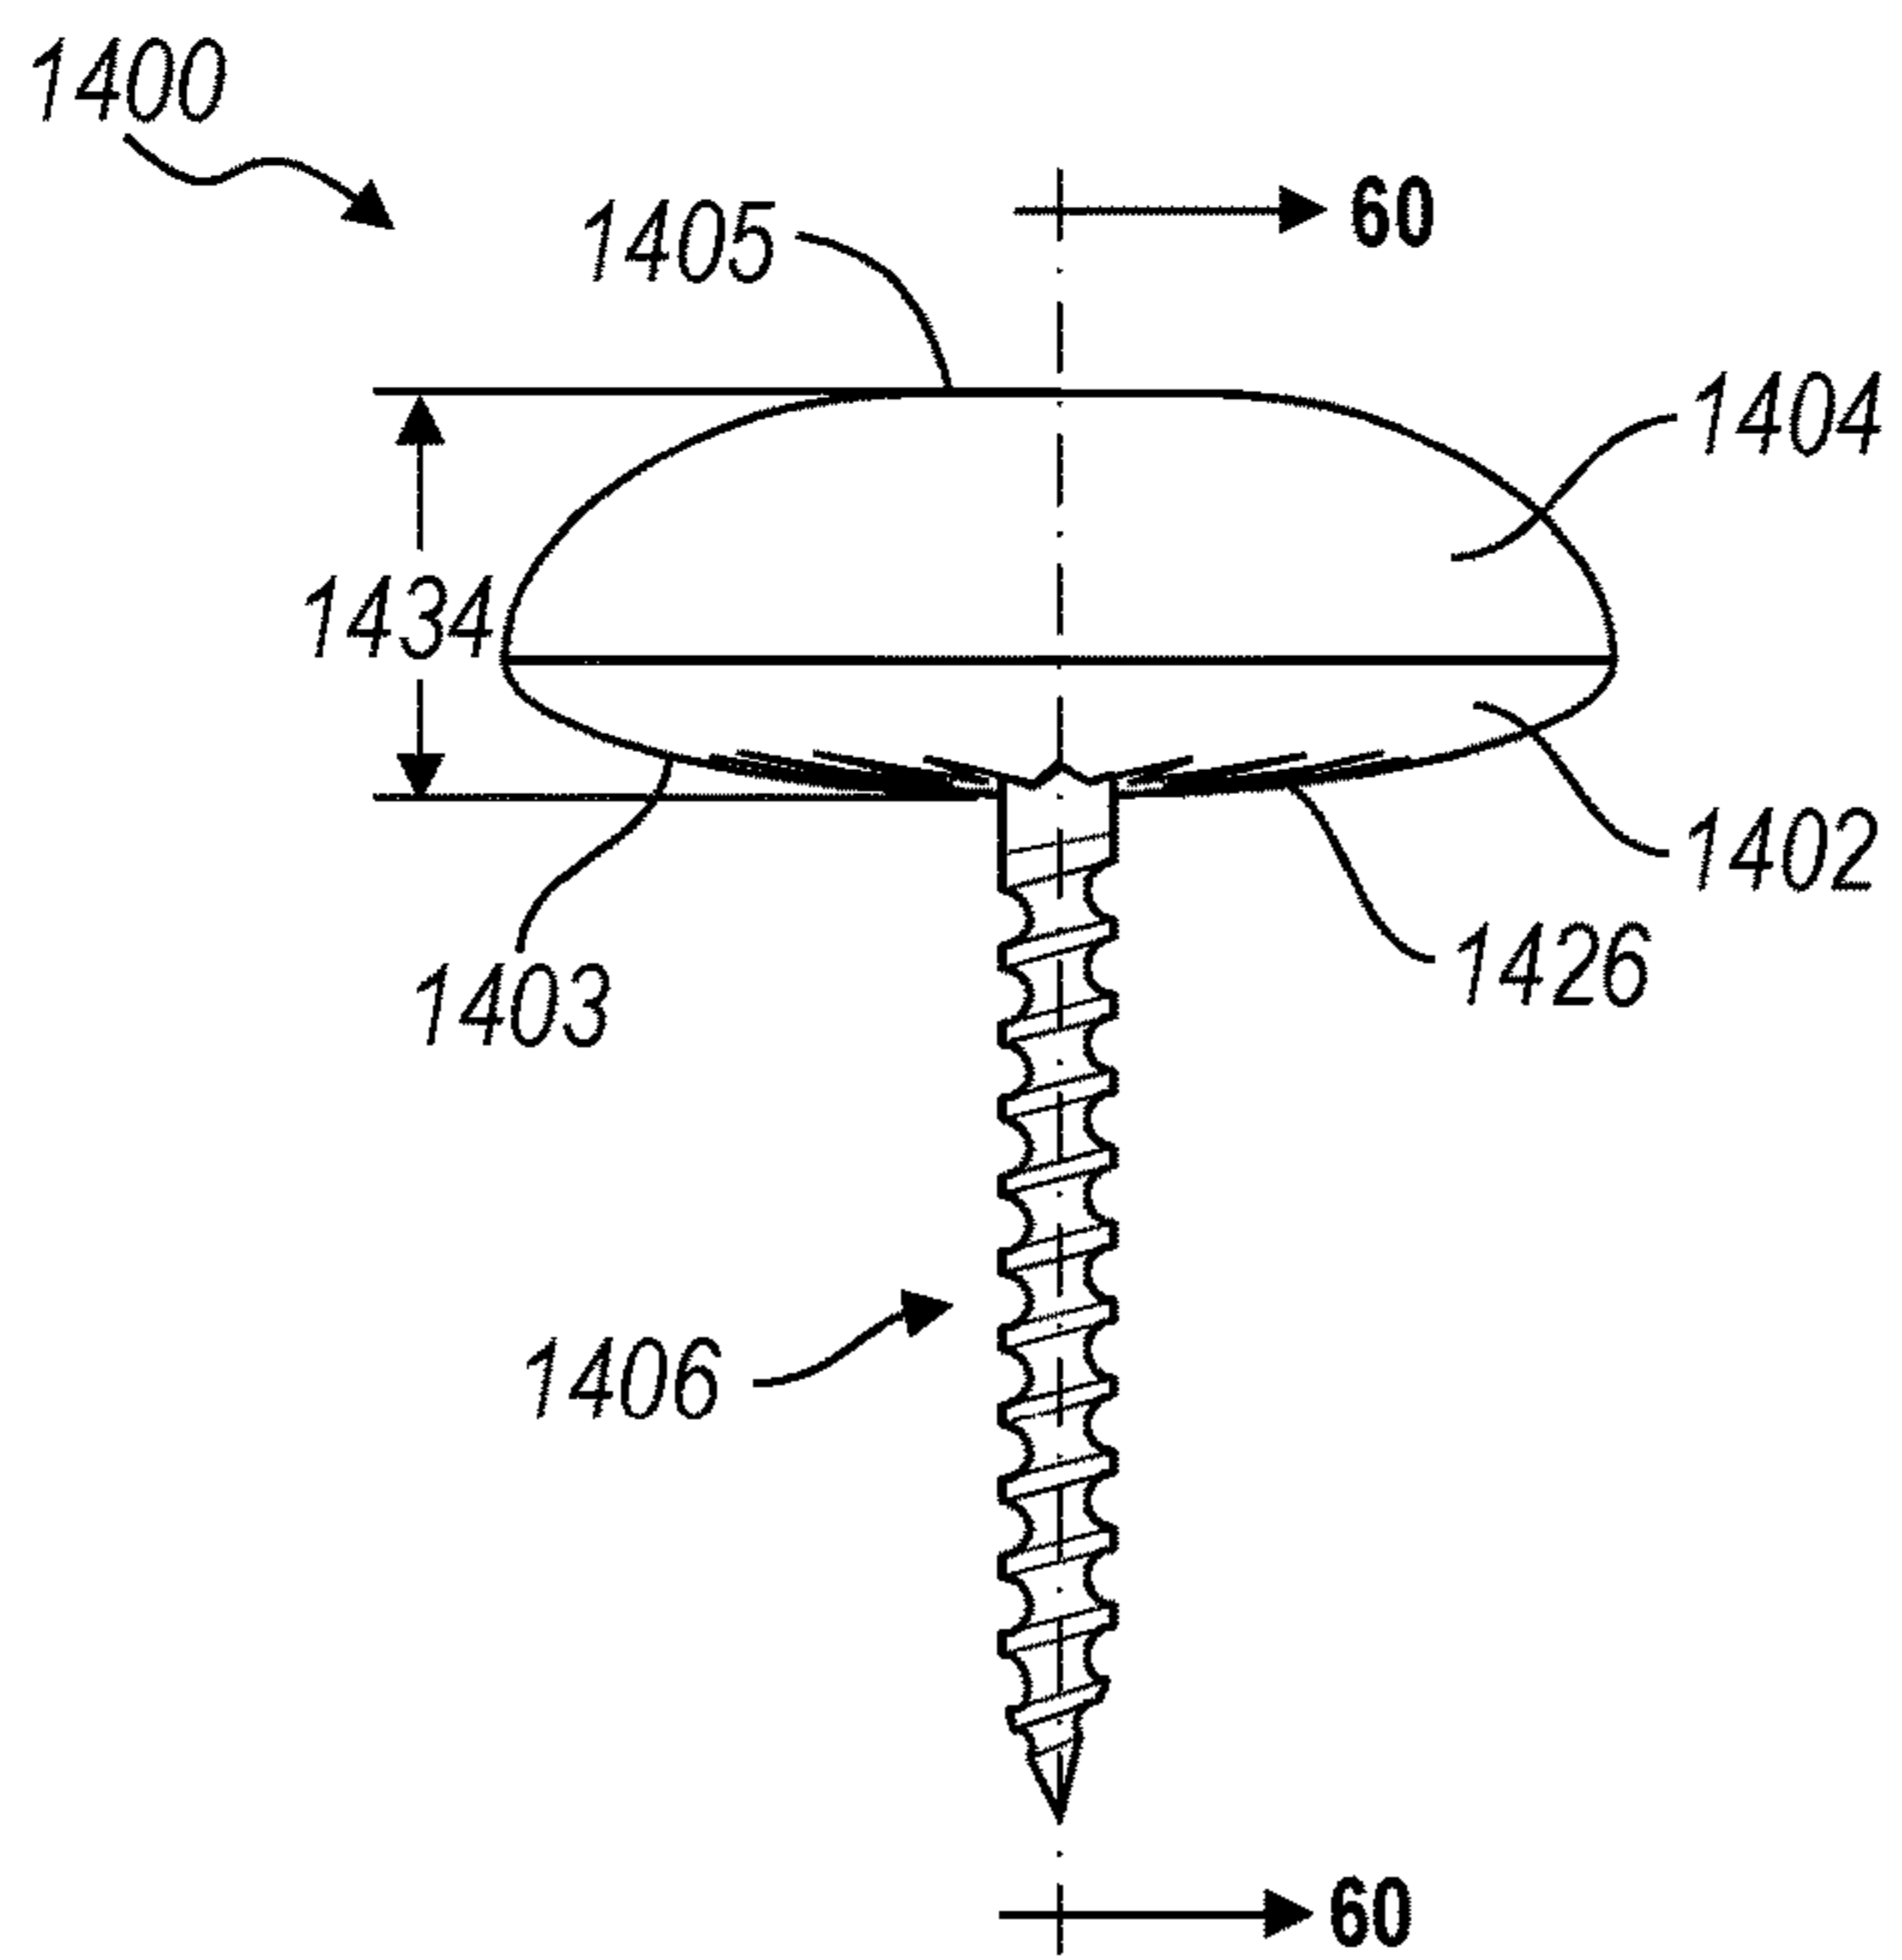


FIG. 59

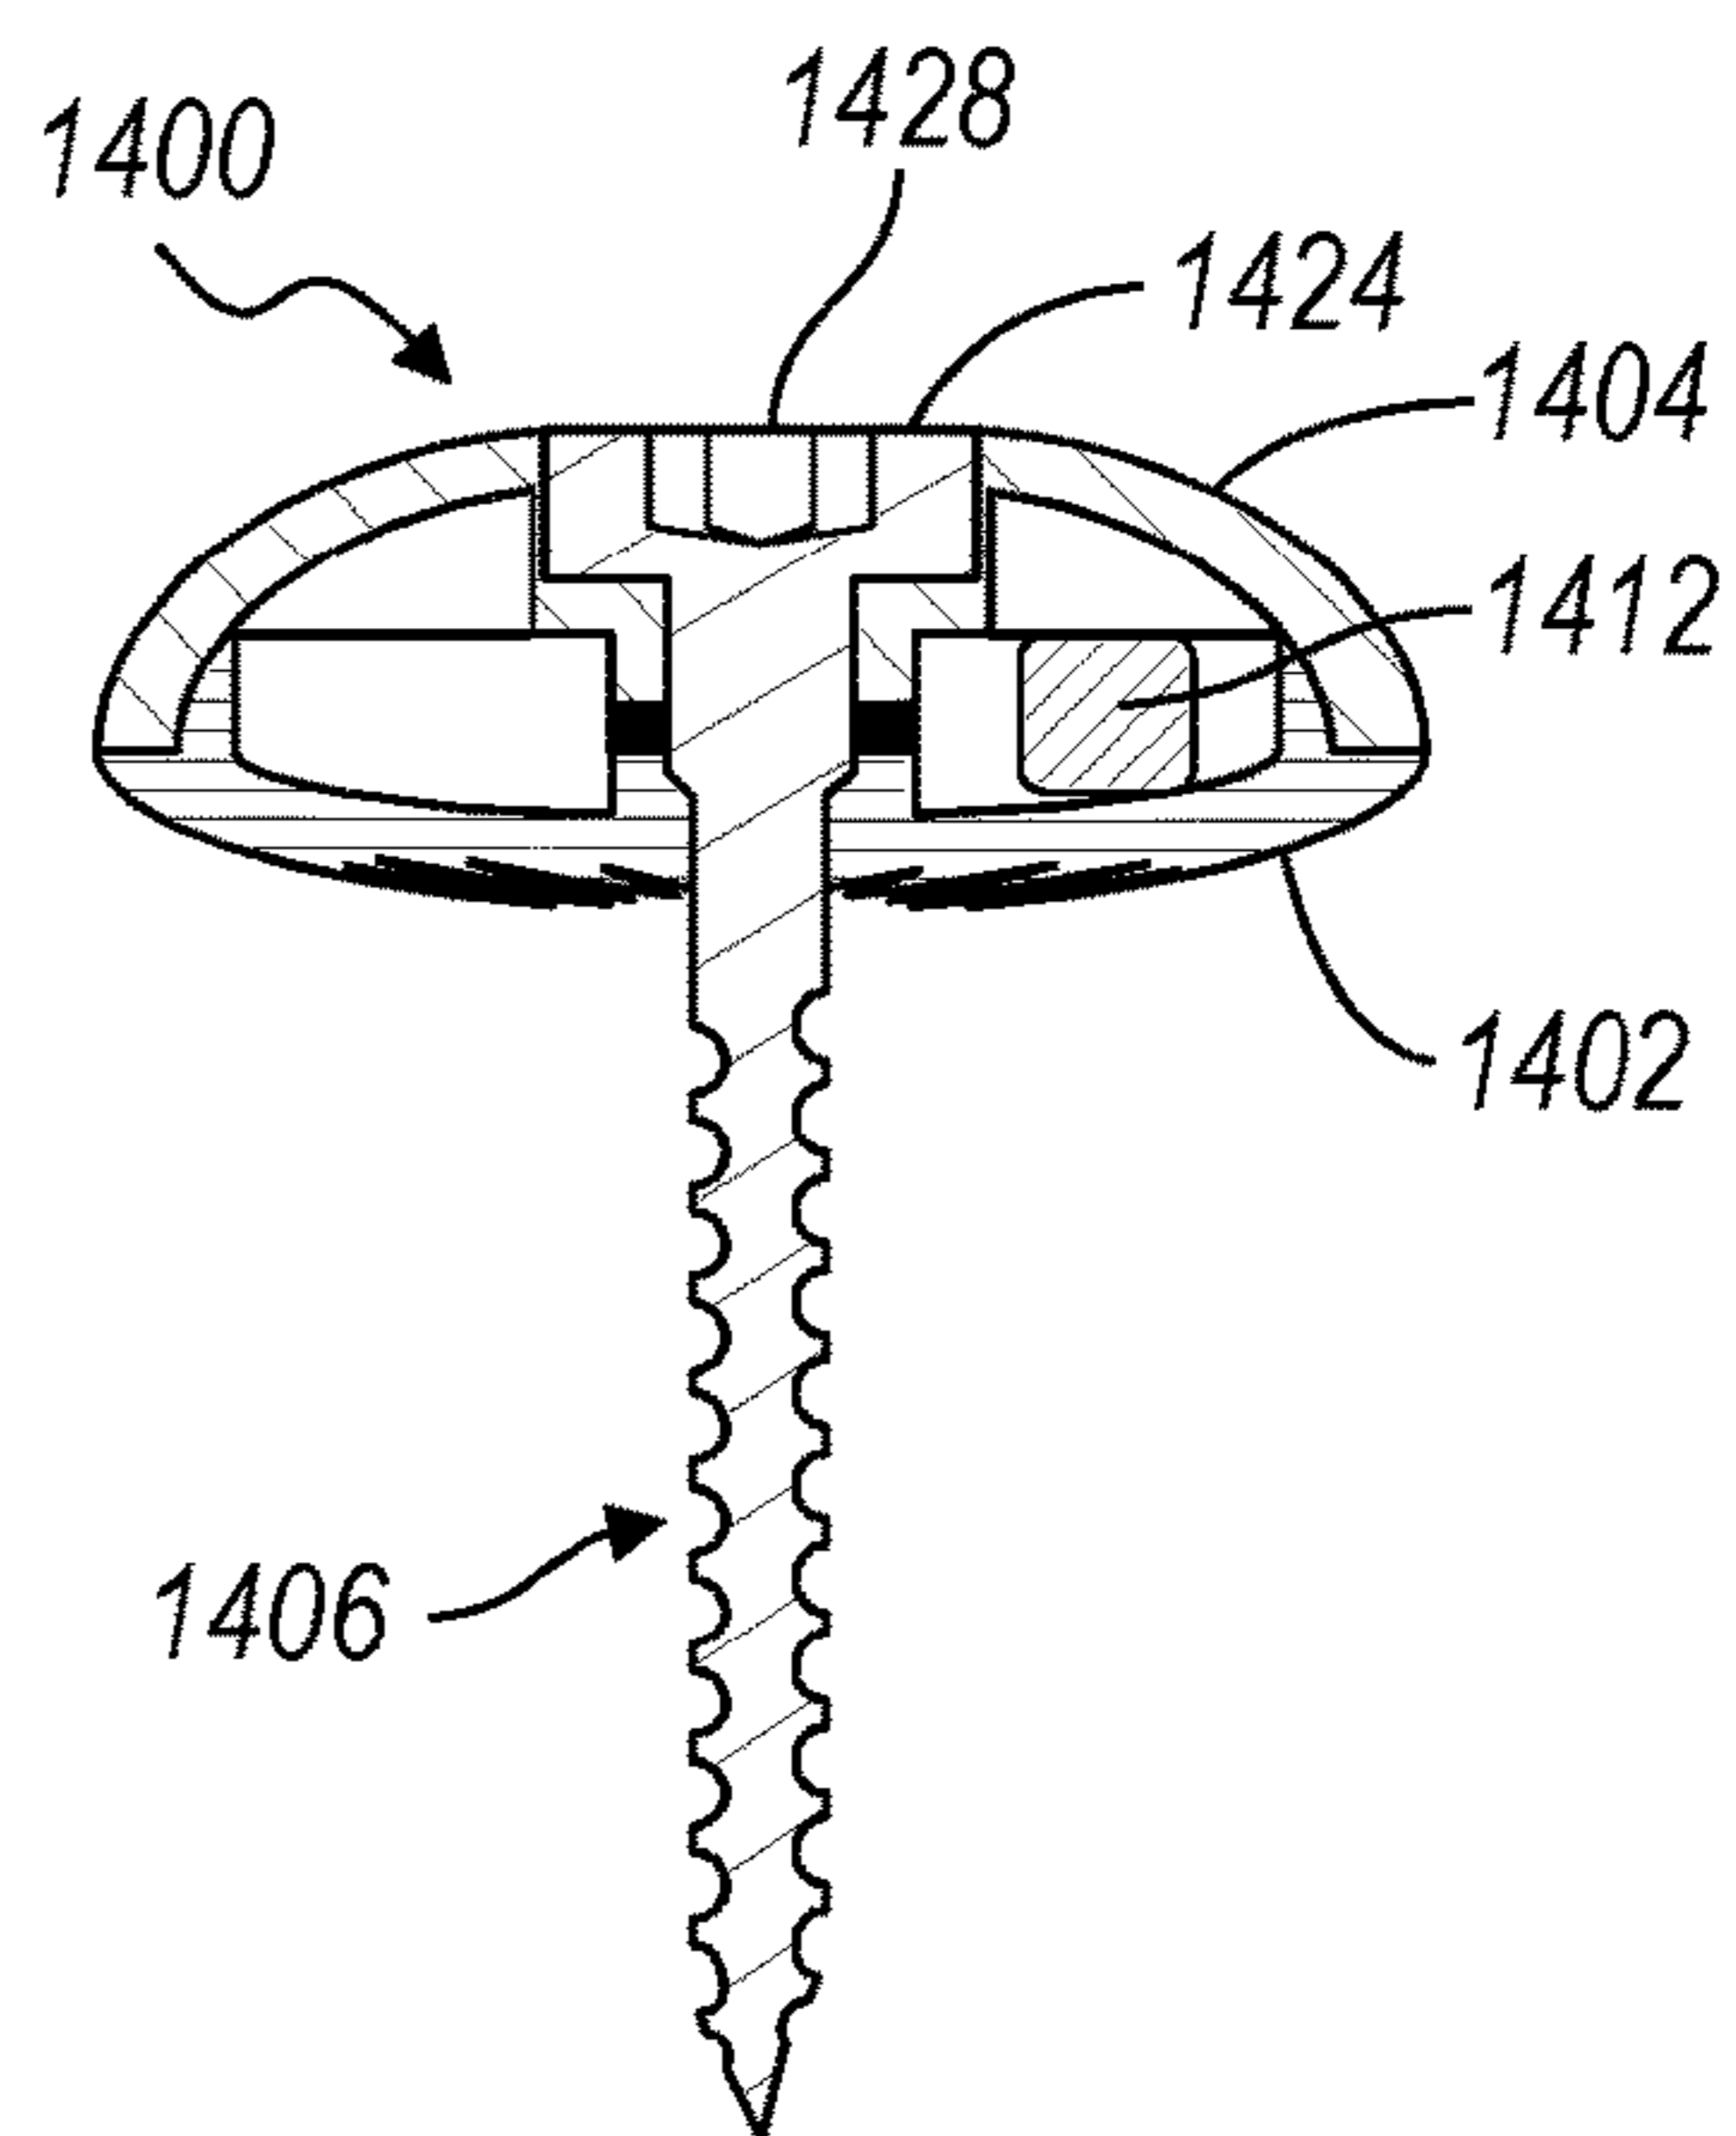


FIG. 60

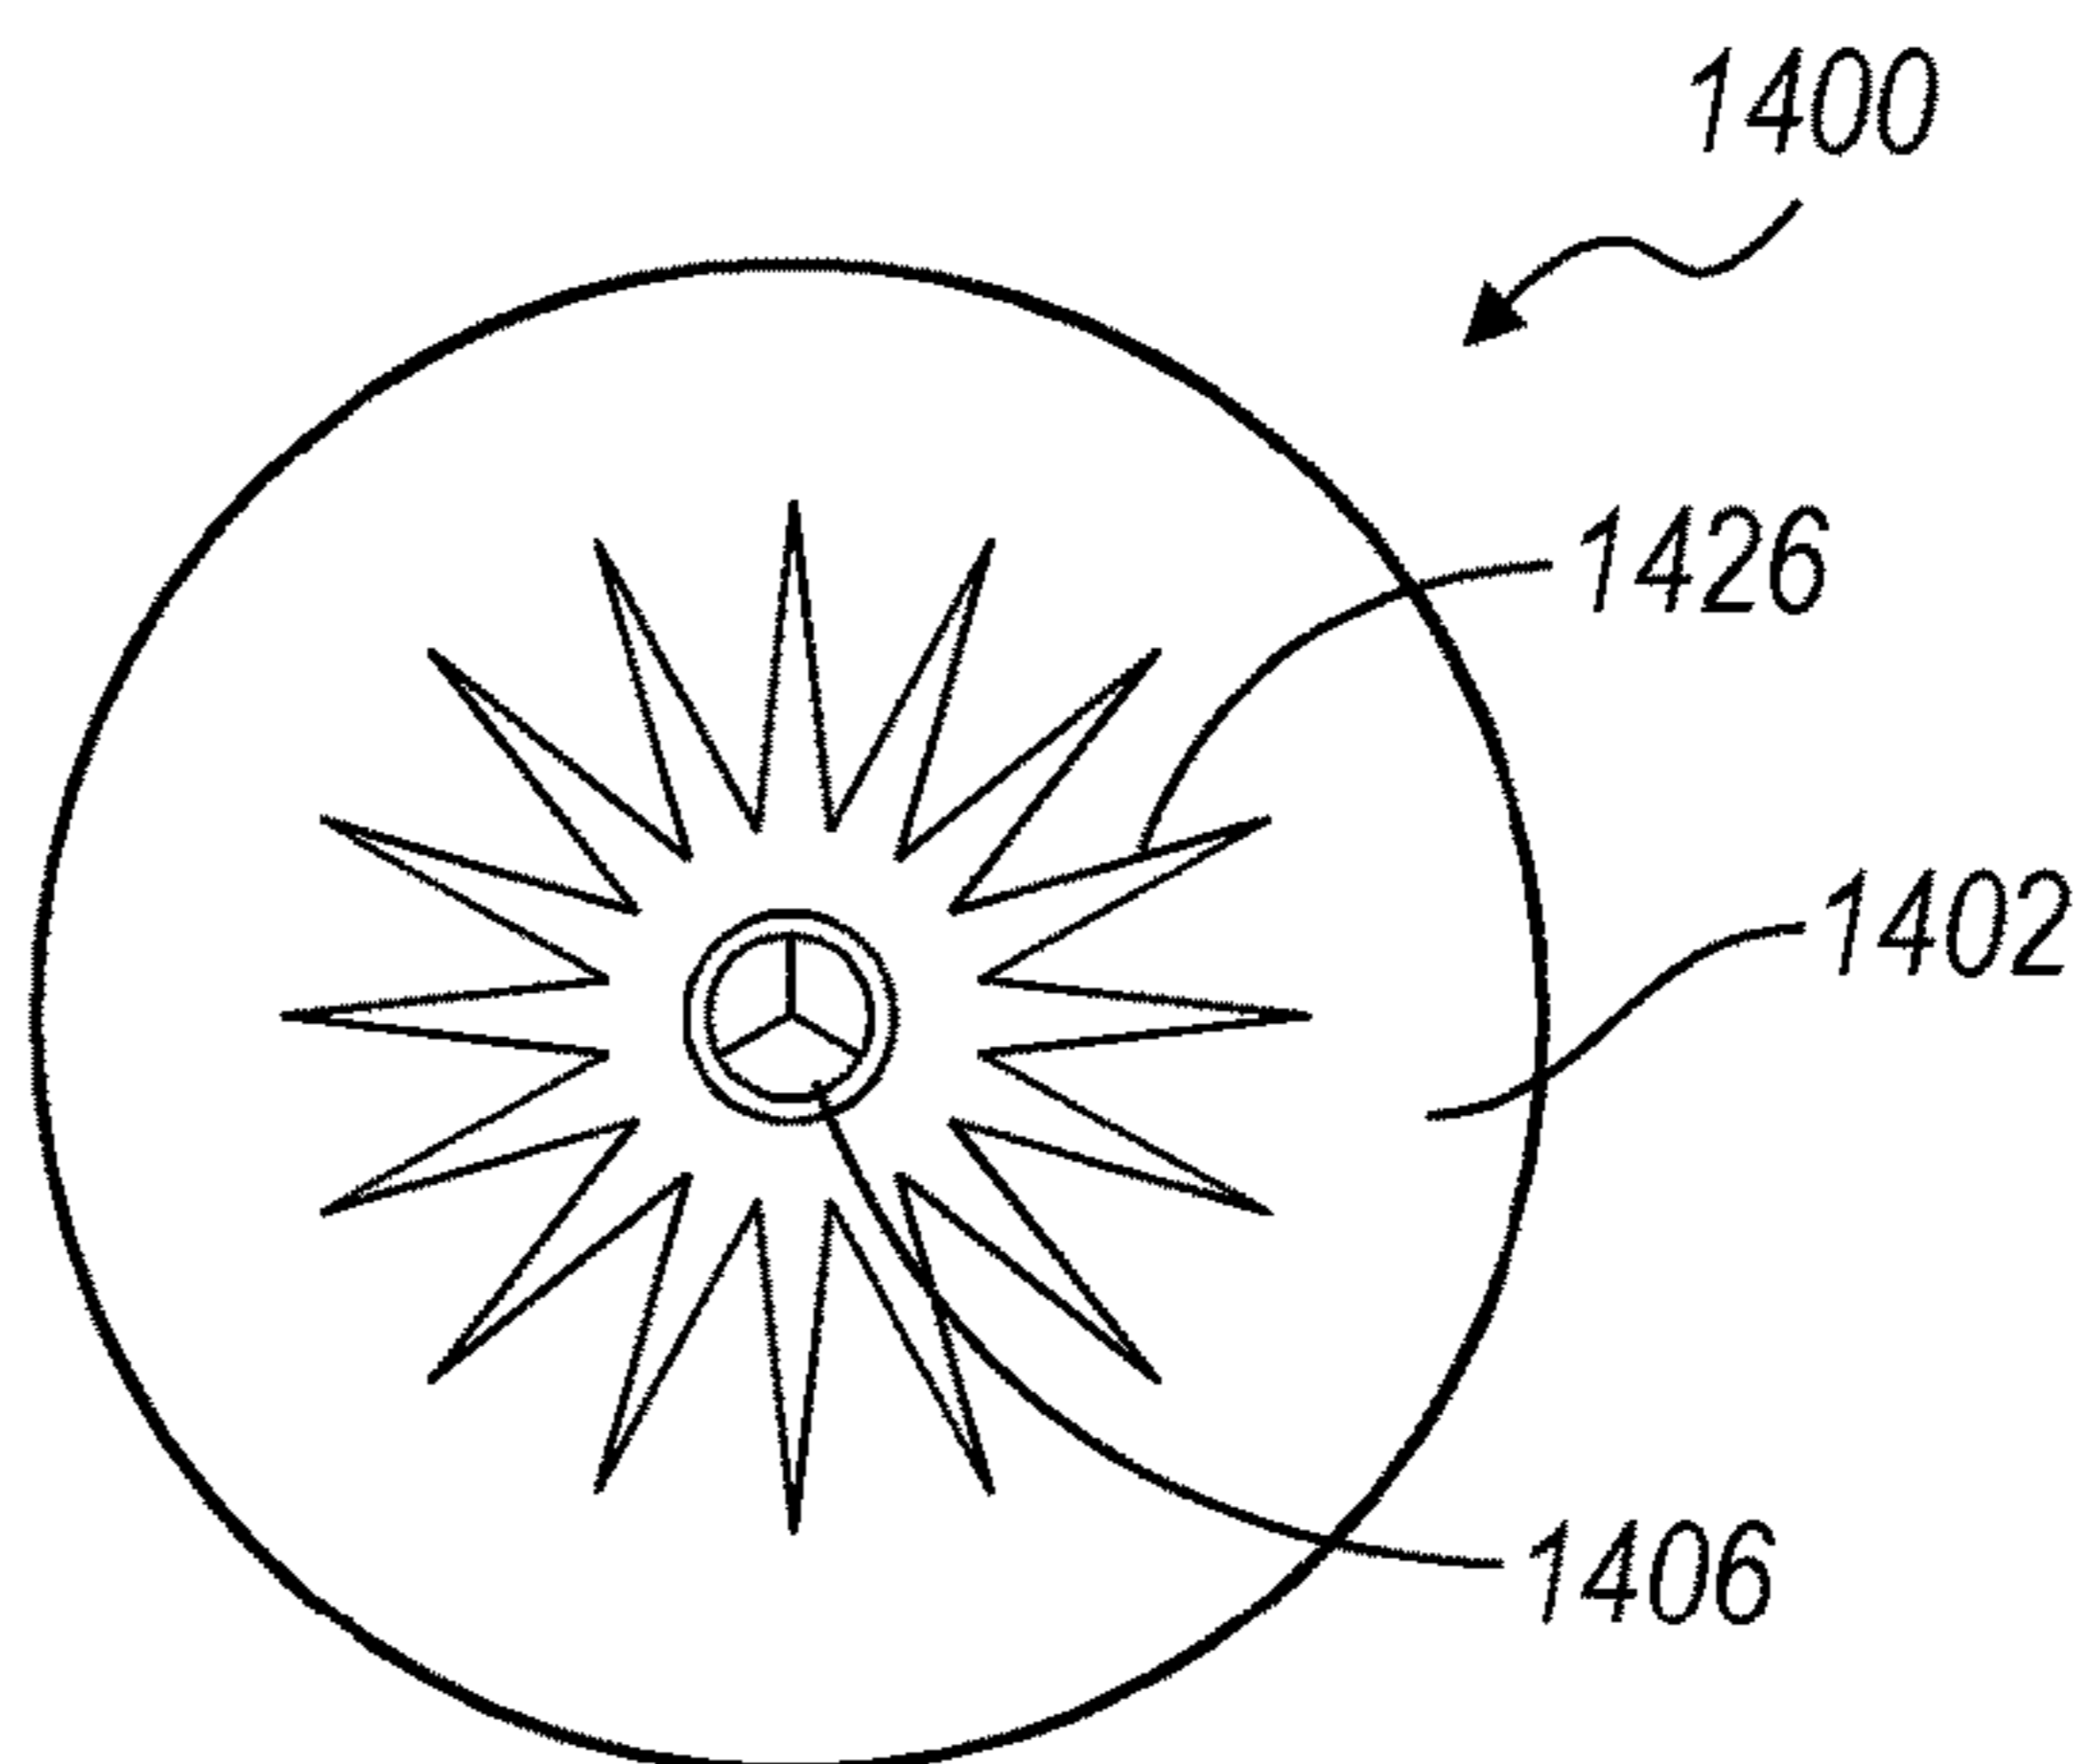


FIG. 61

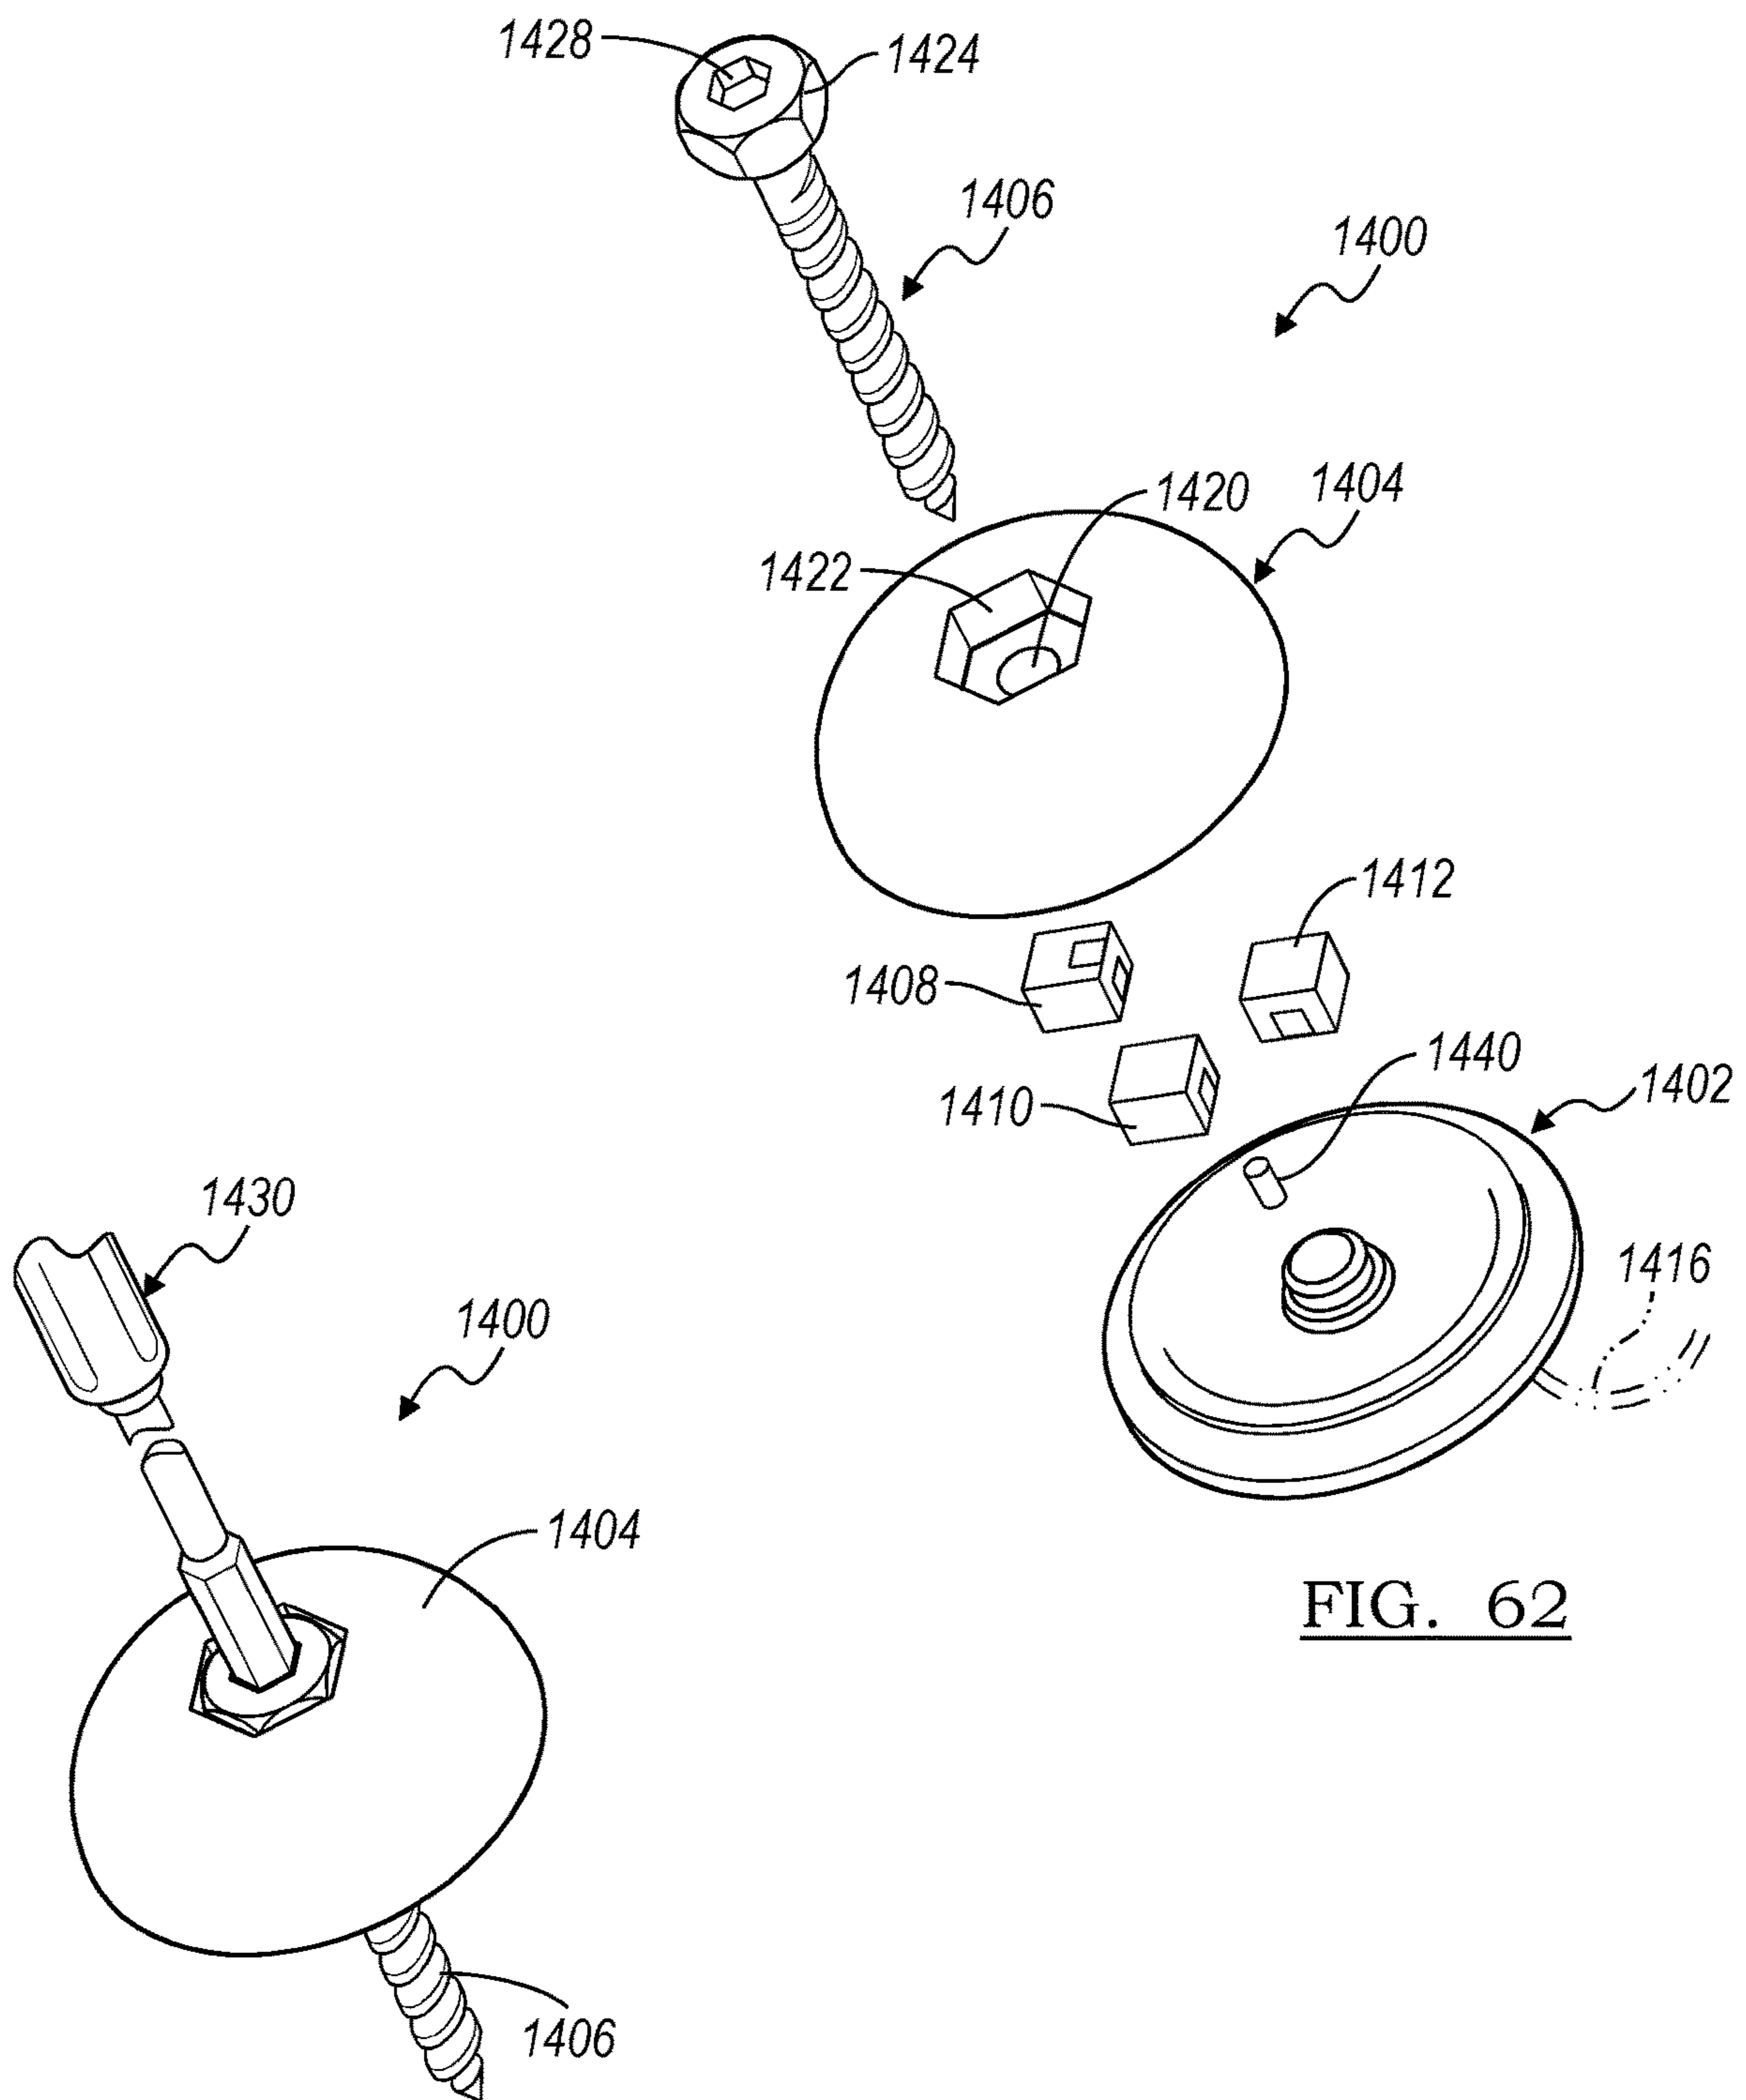


FIG. 62

FIG. 63

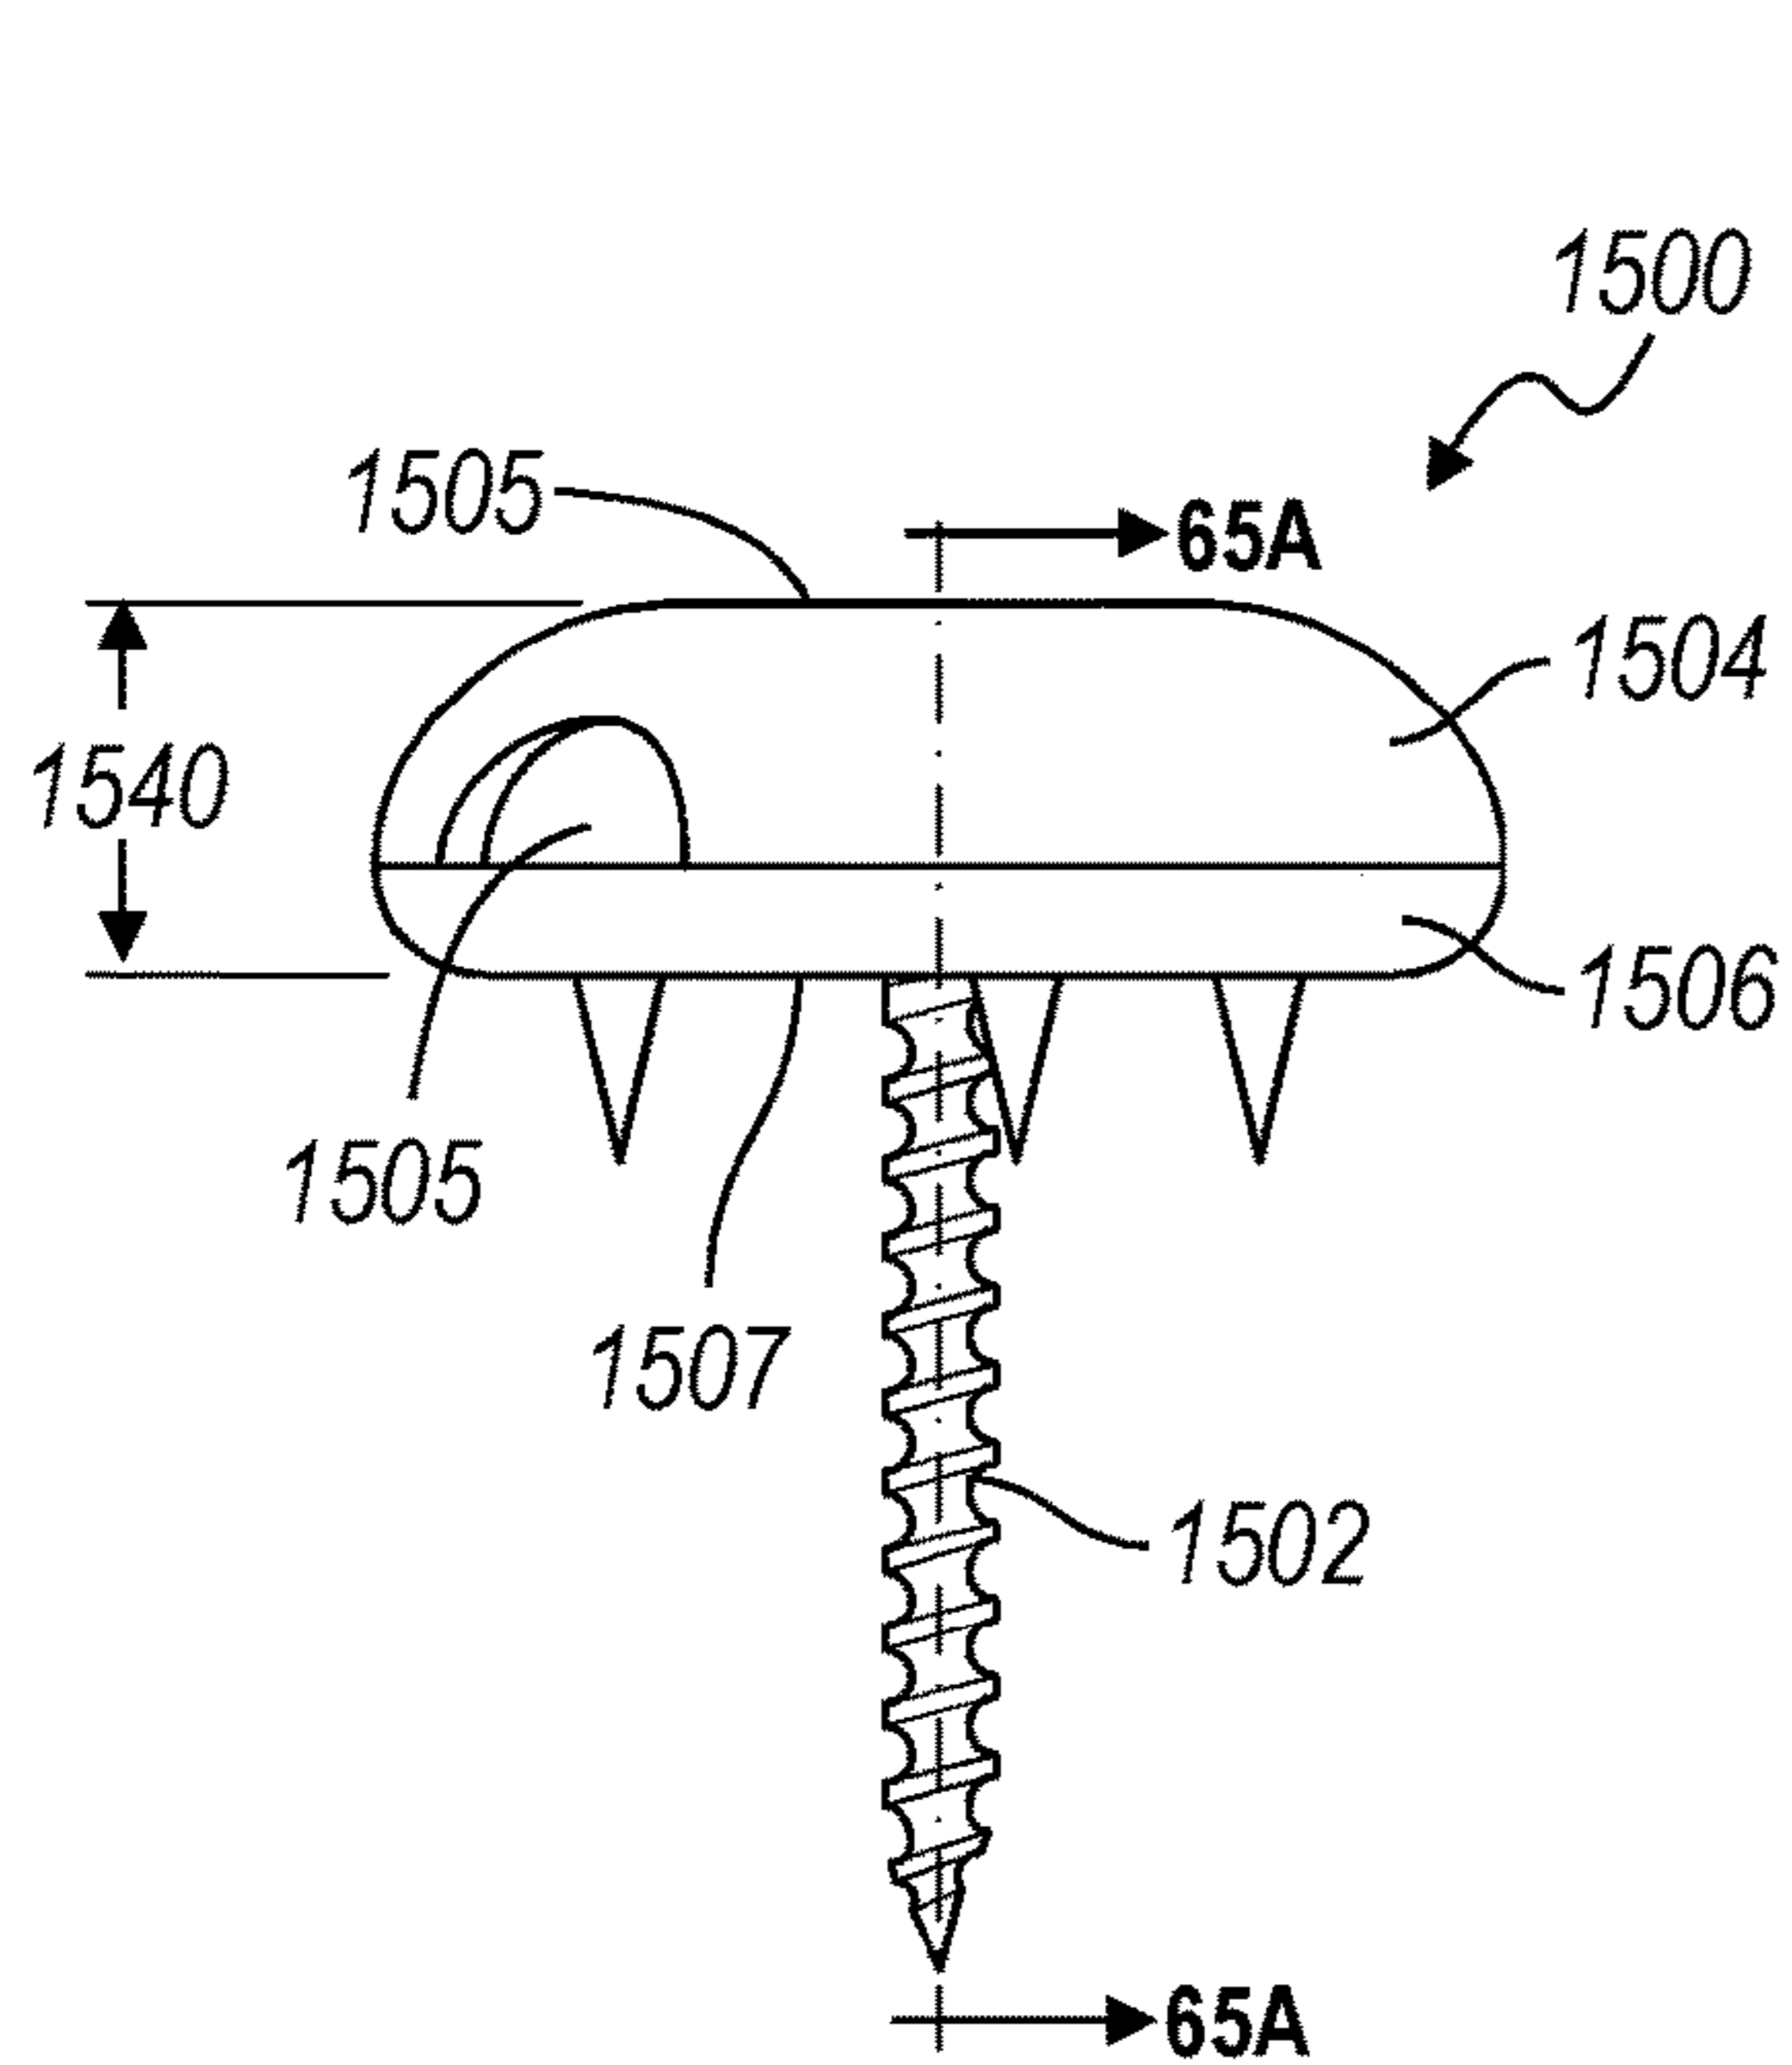


FIG. 64

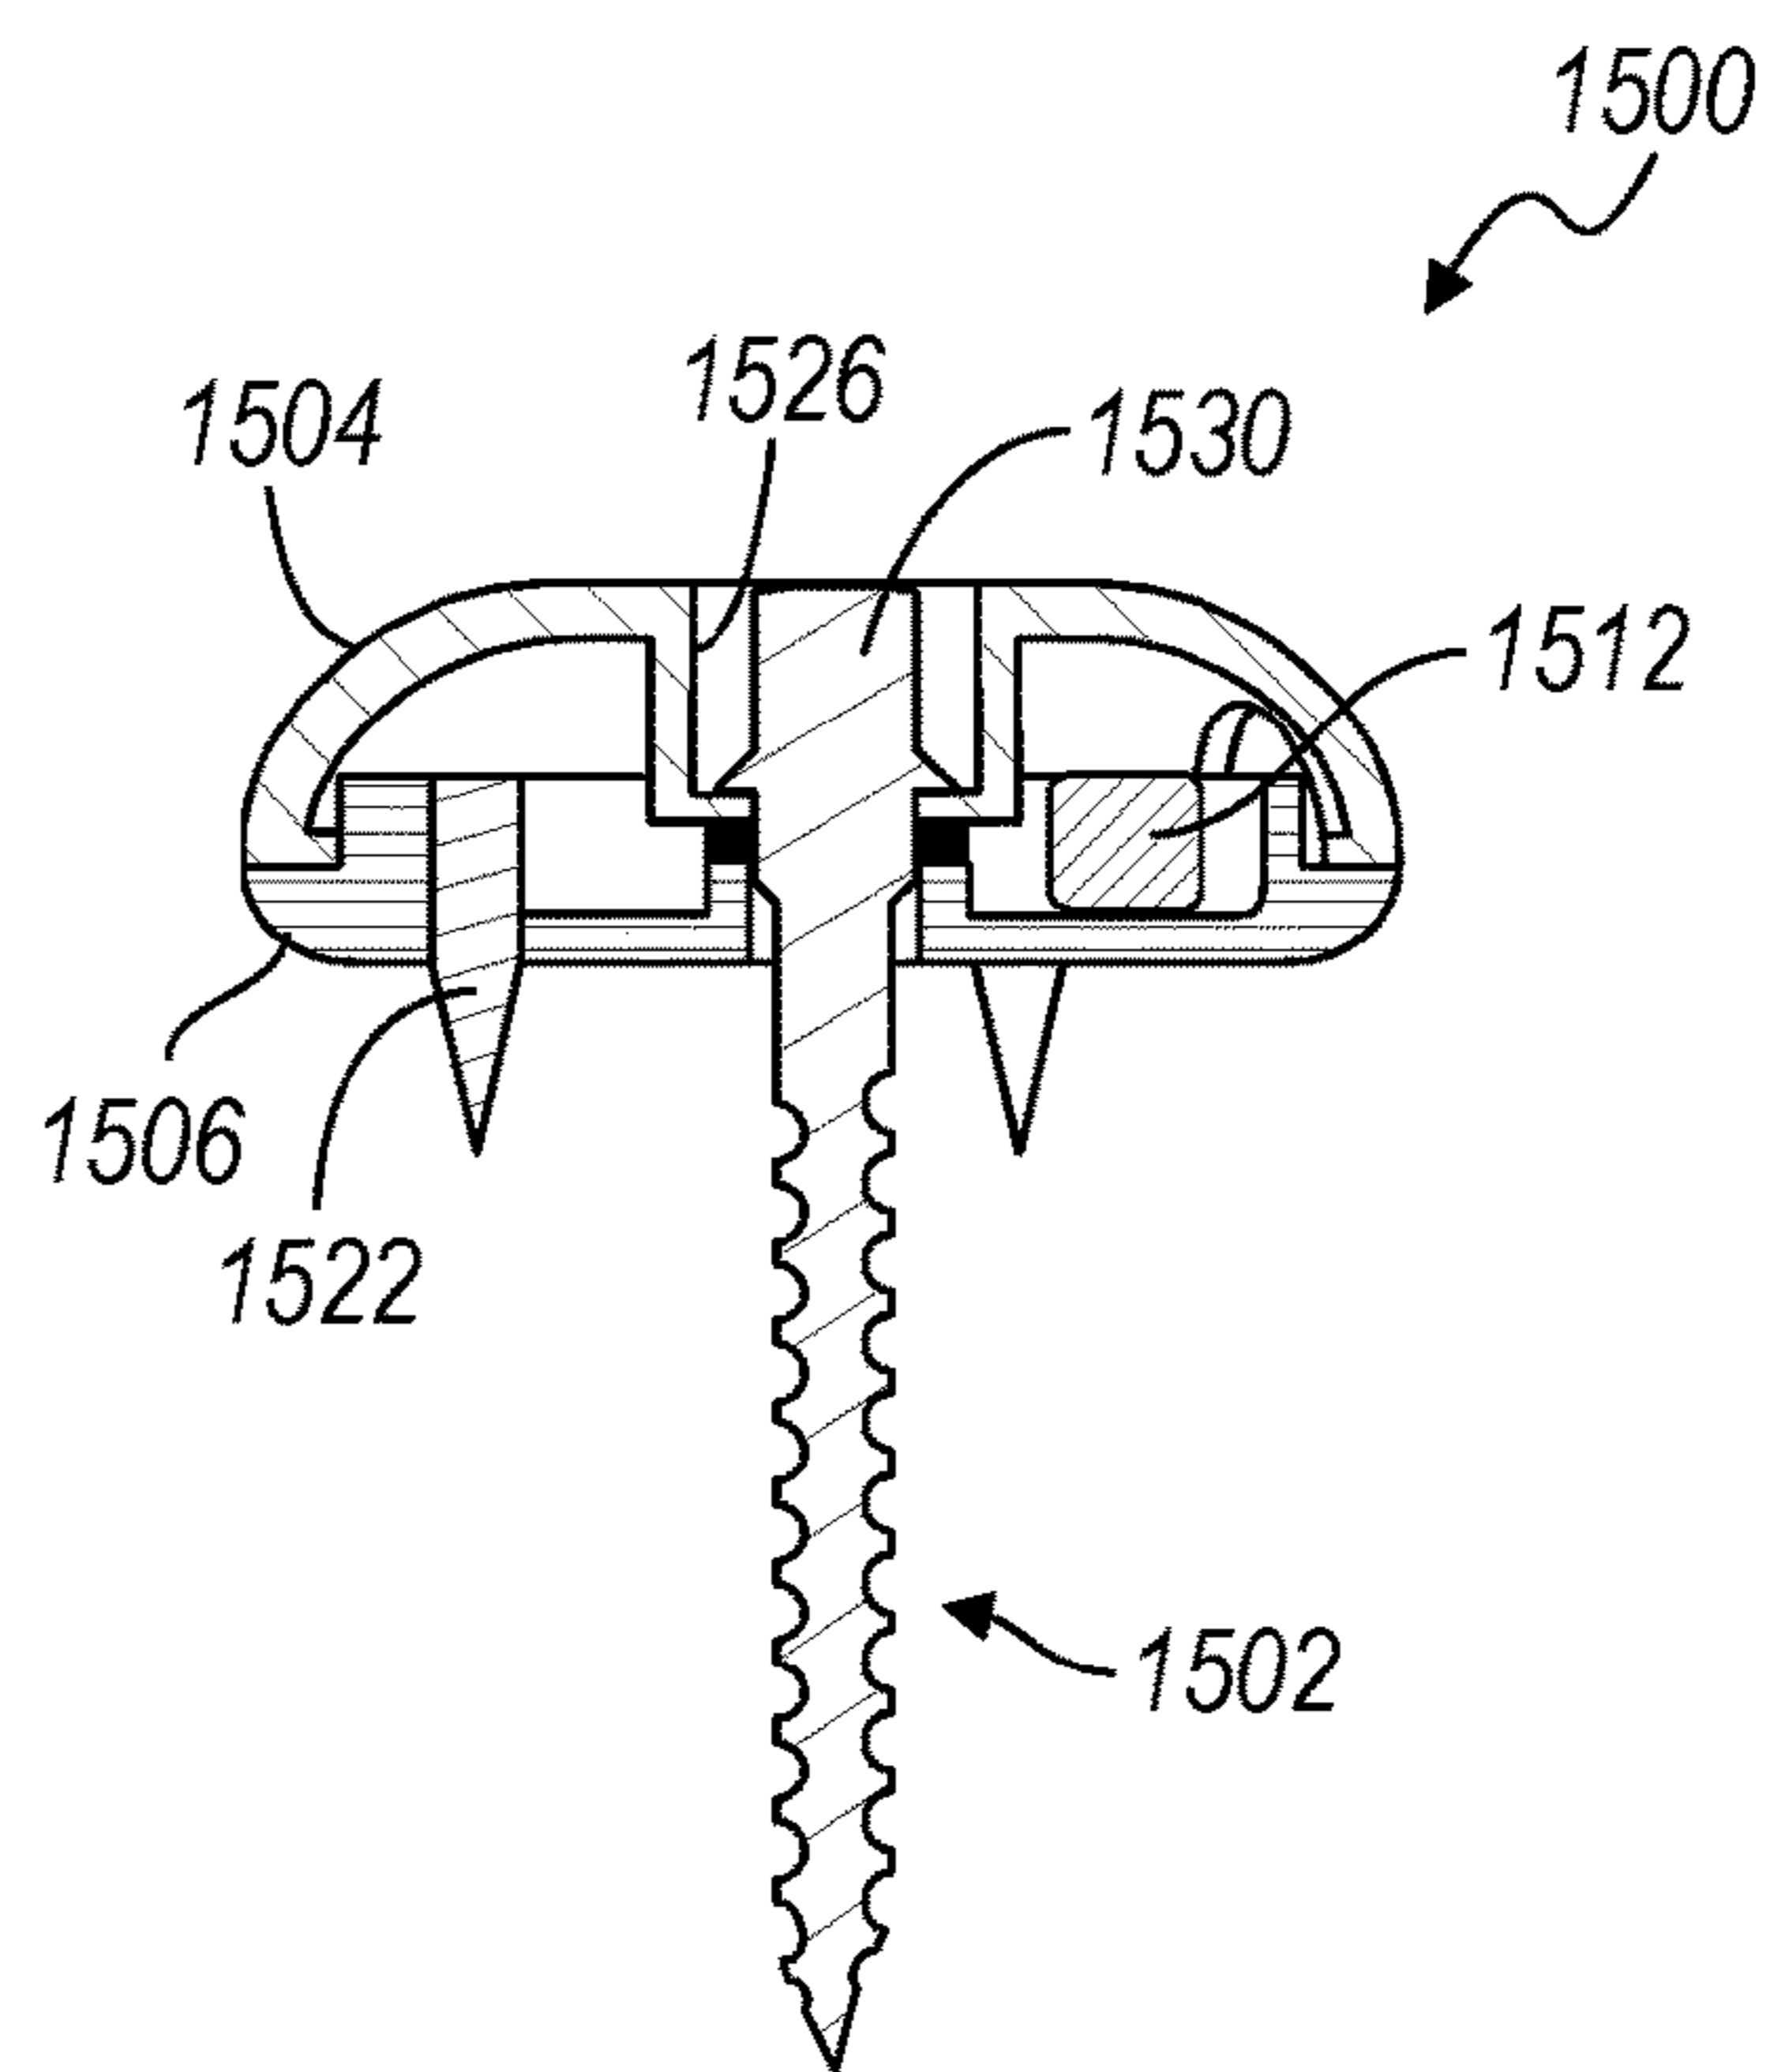


FIG. 65A

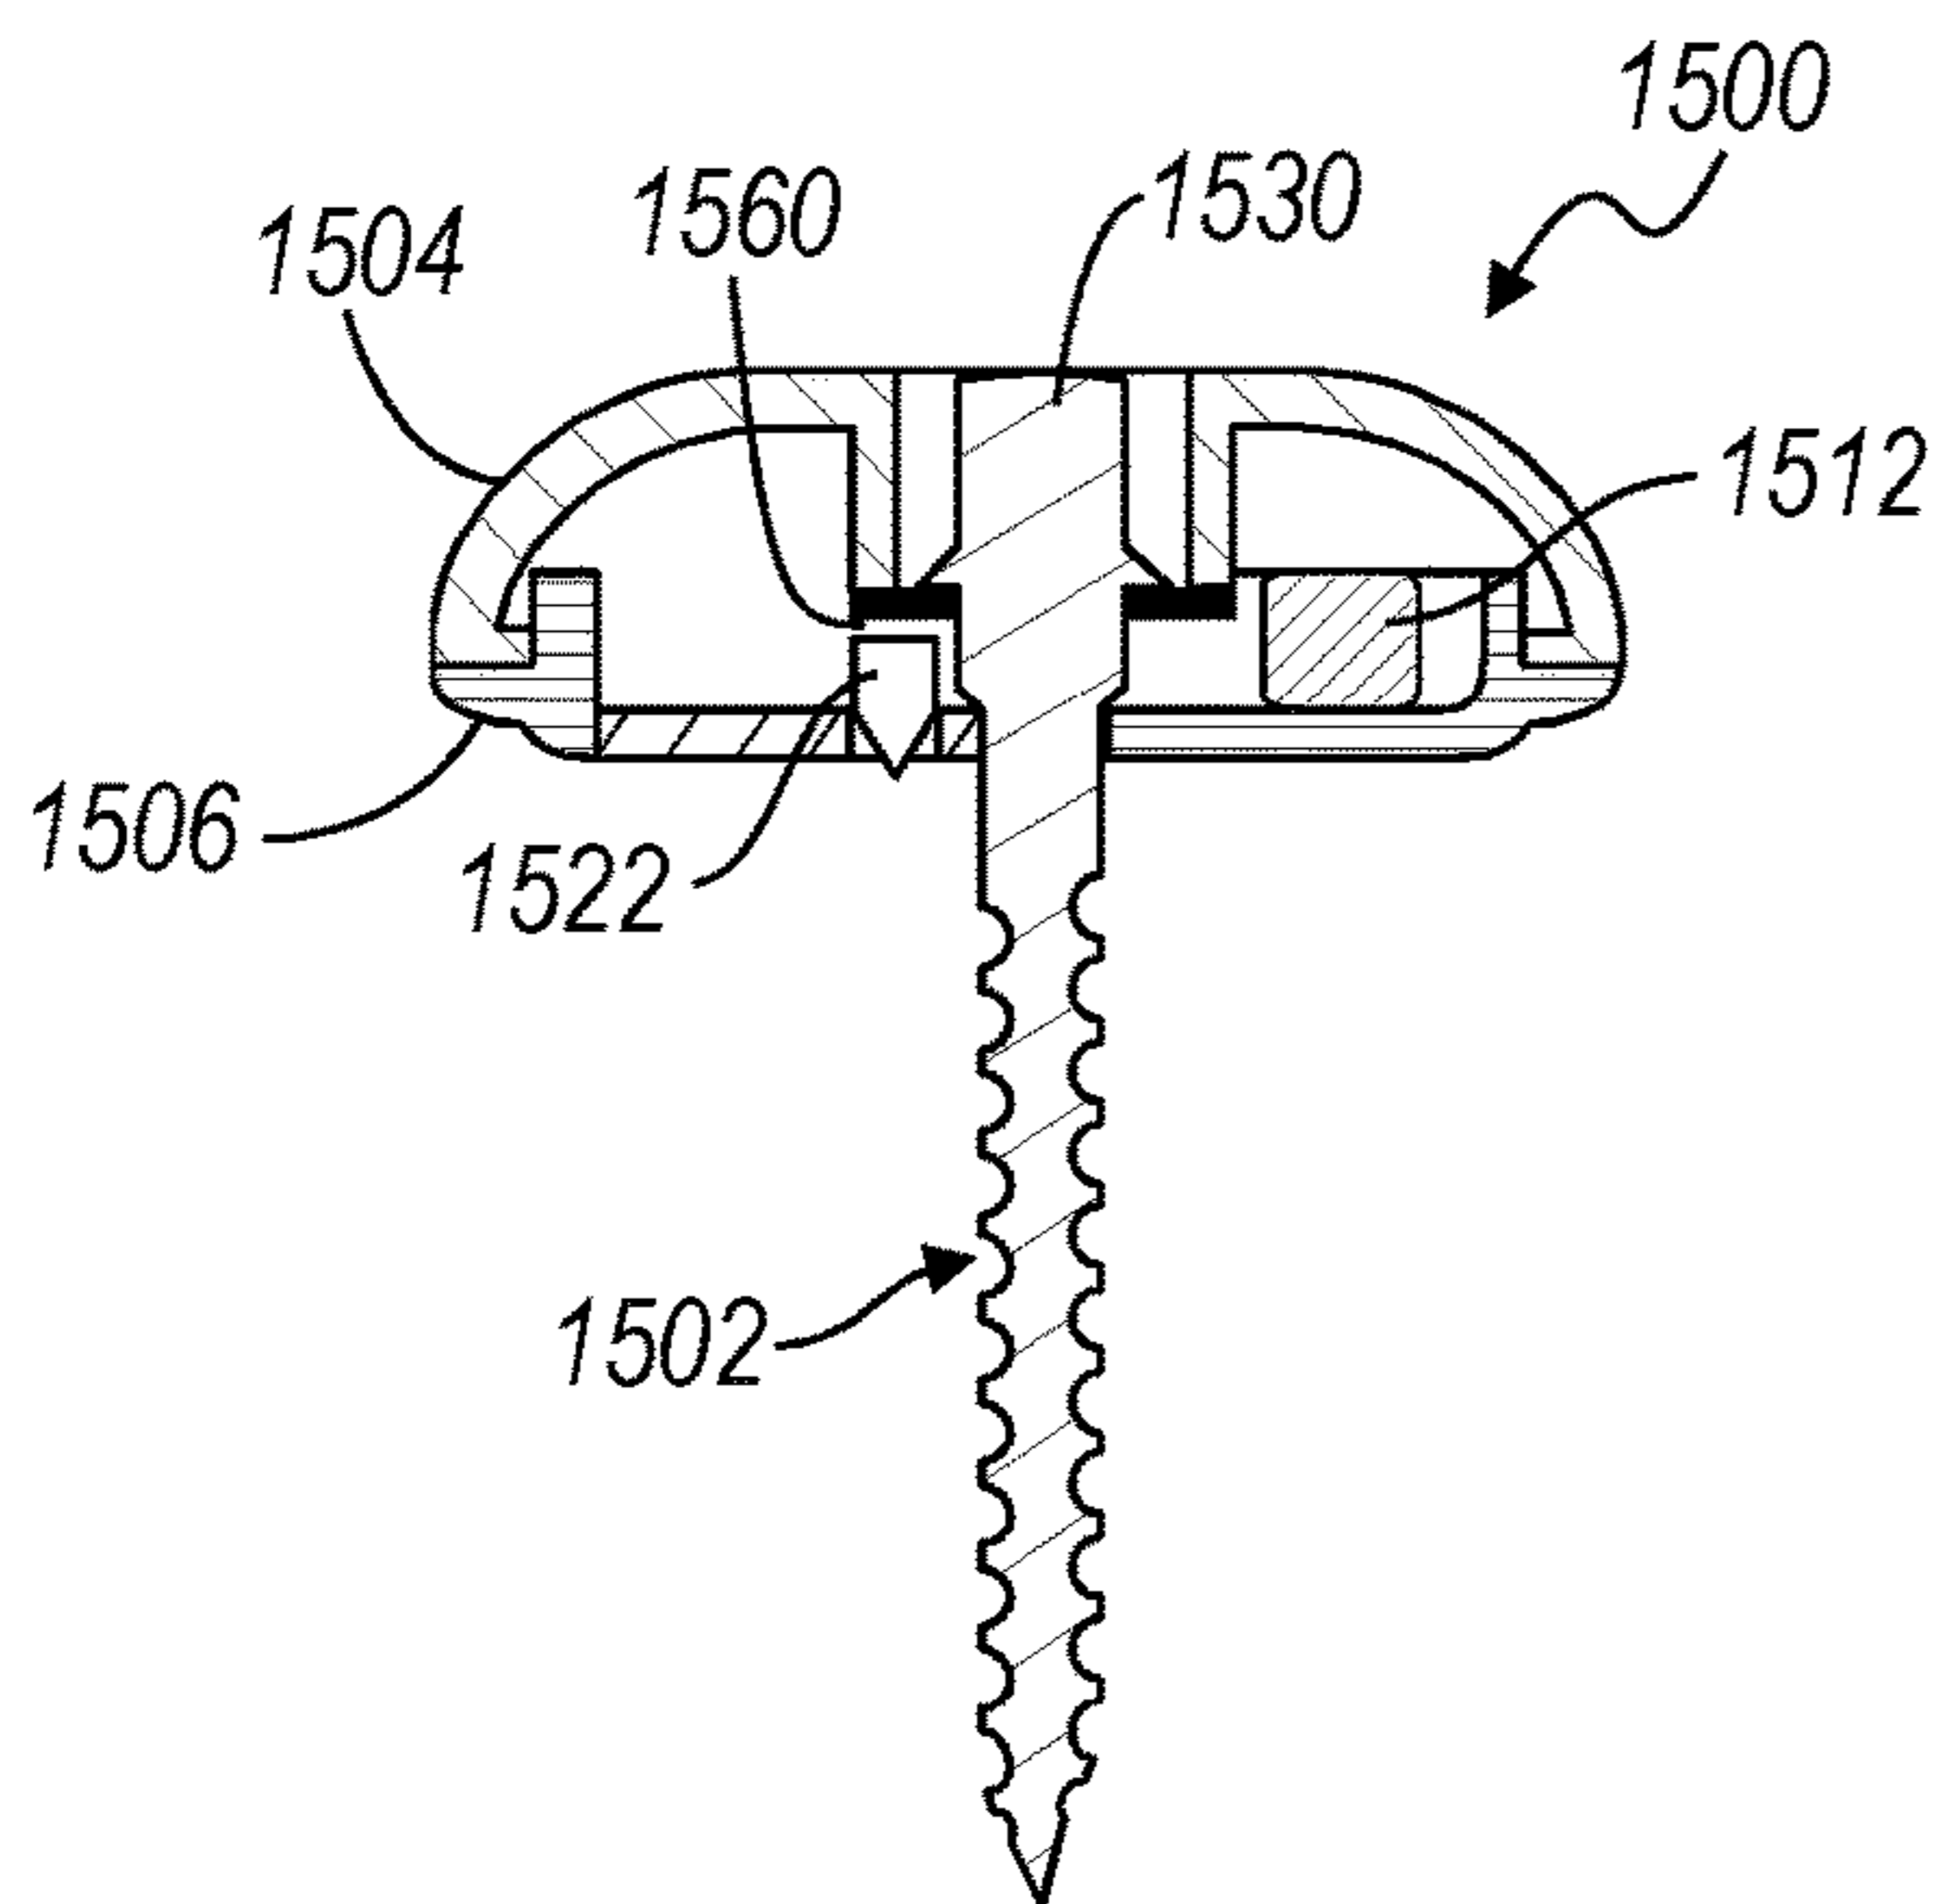


FIG. 65B

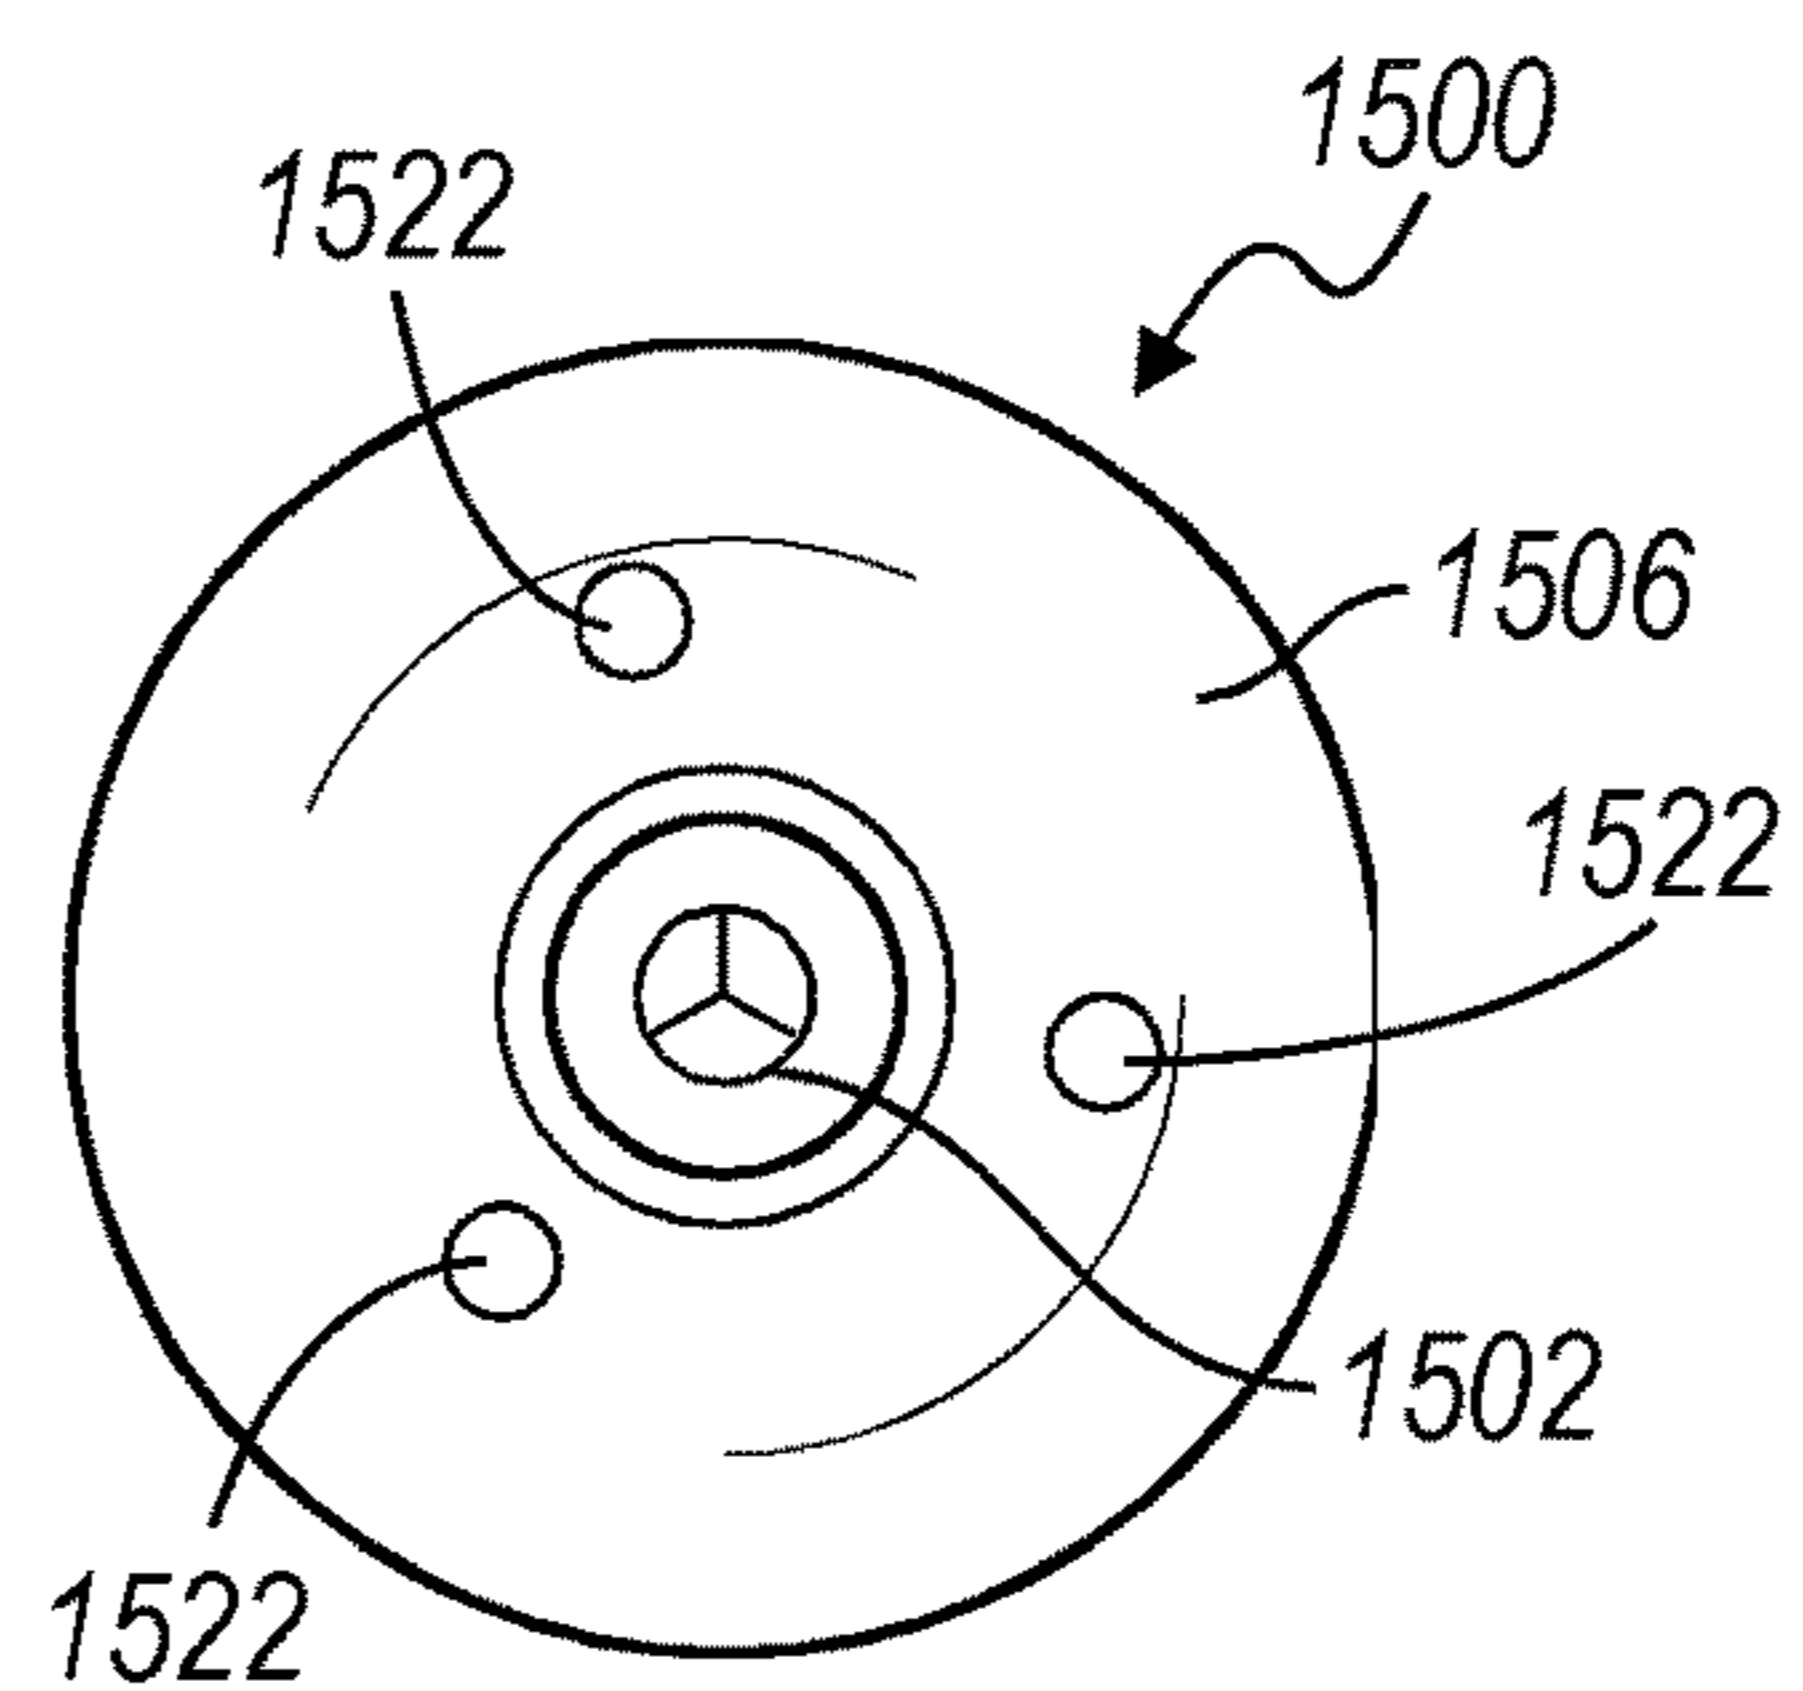


FIG. 66

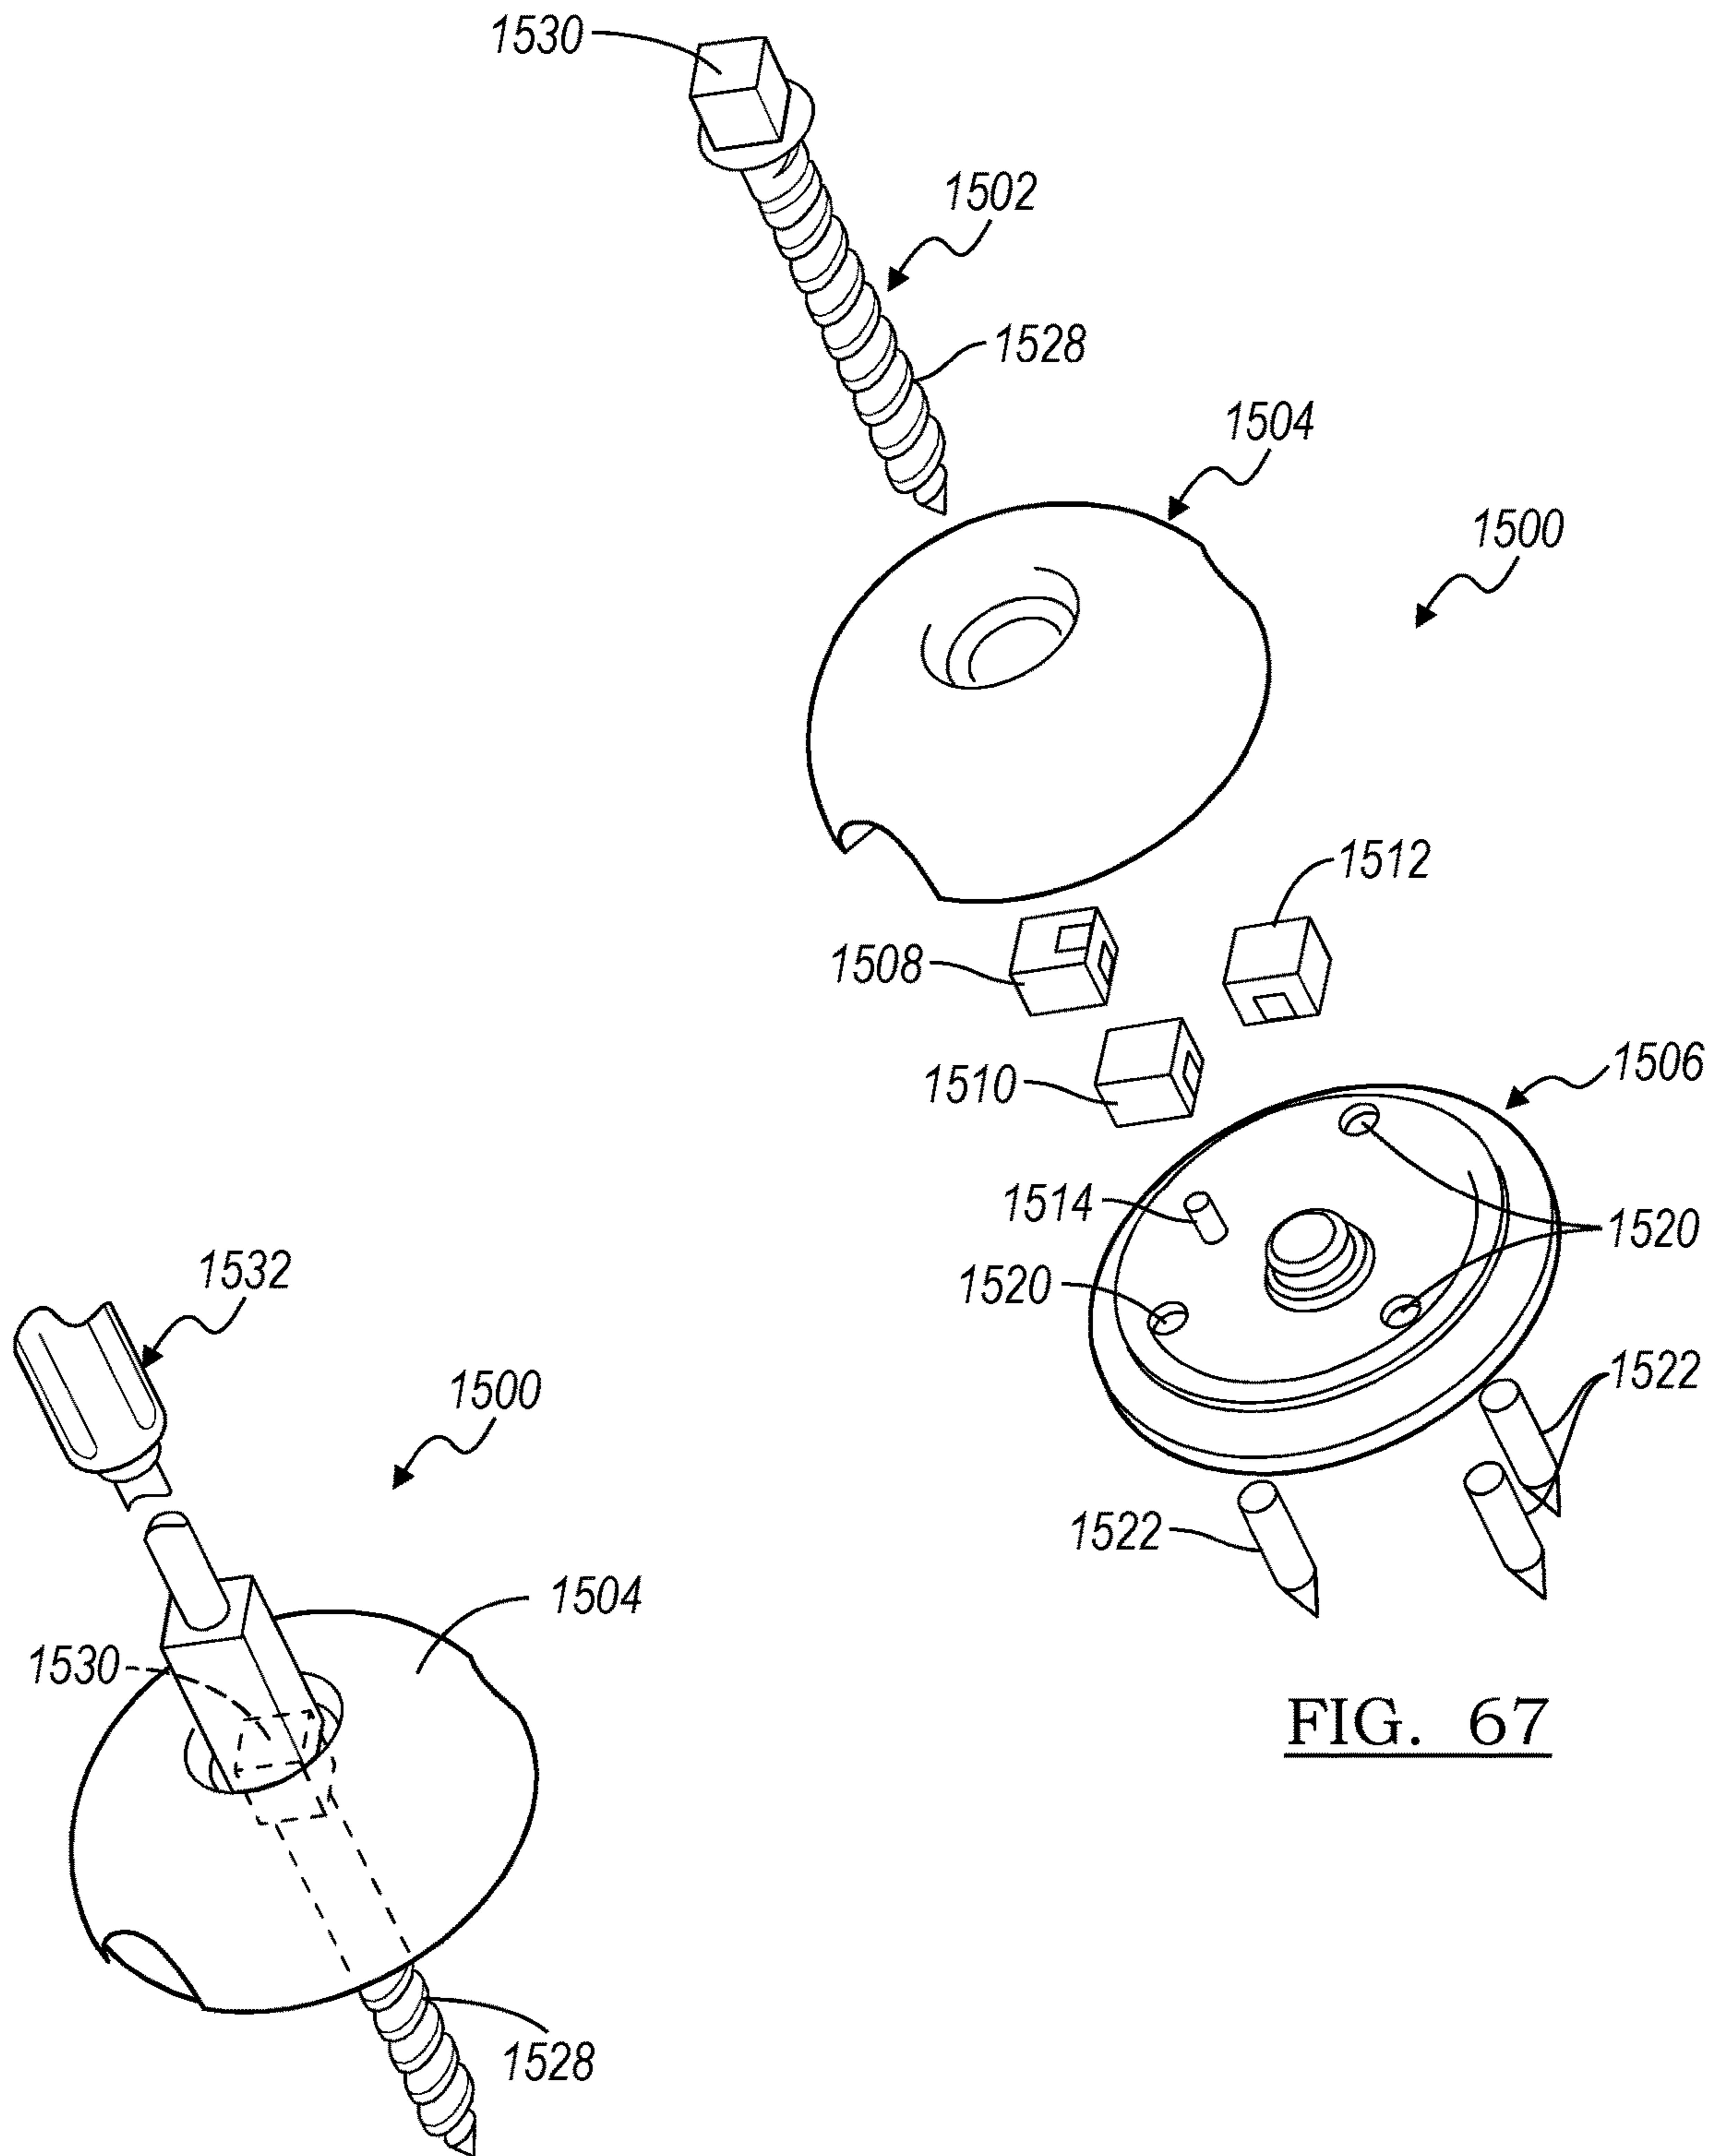


FIG. 67

FIG. 68

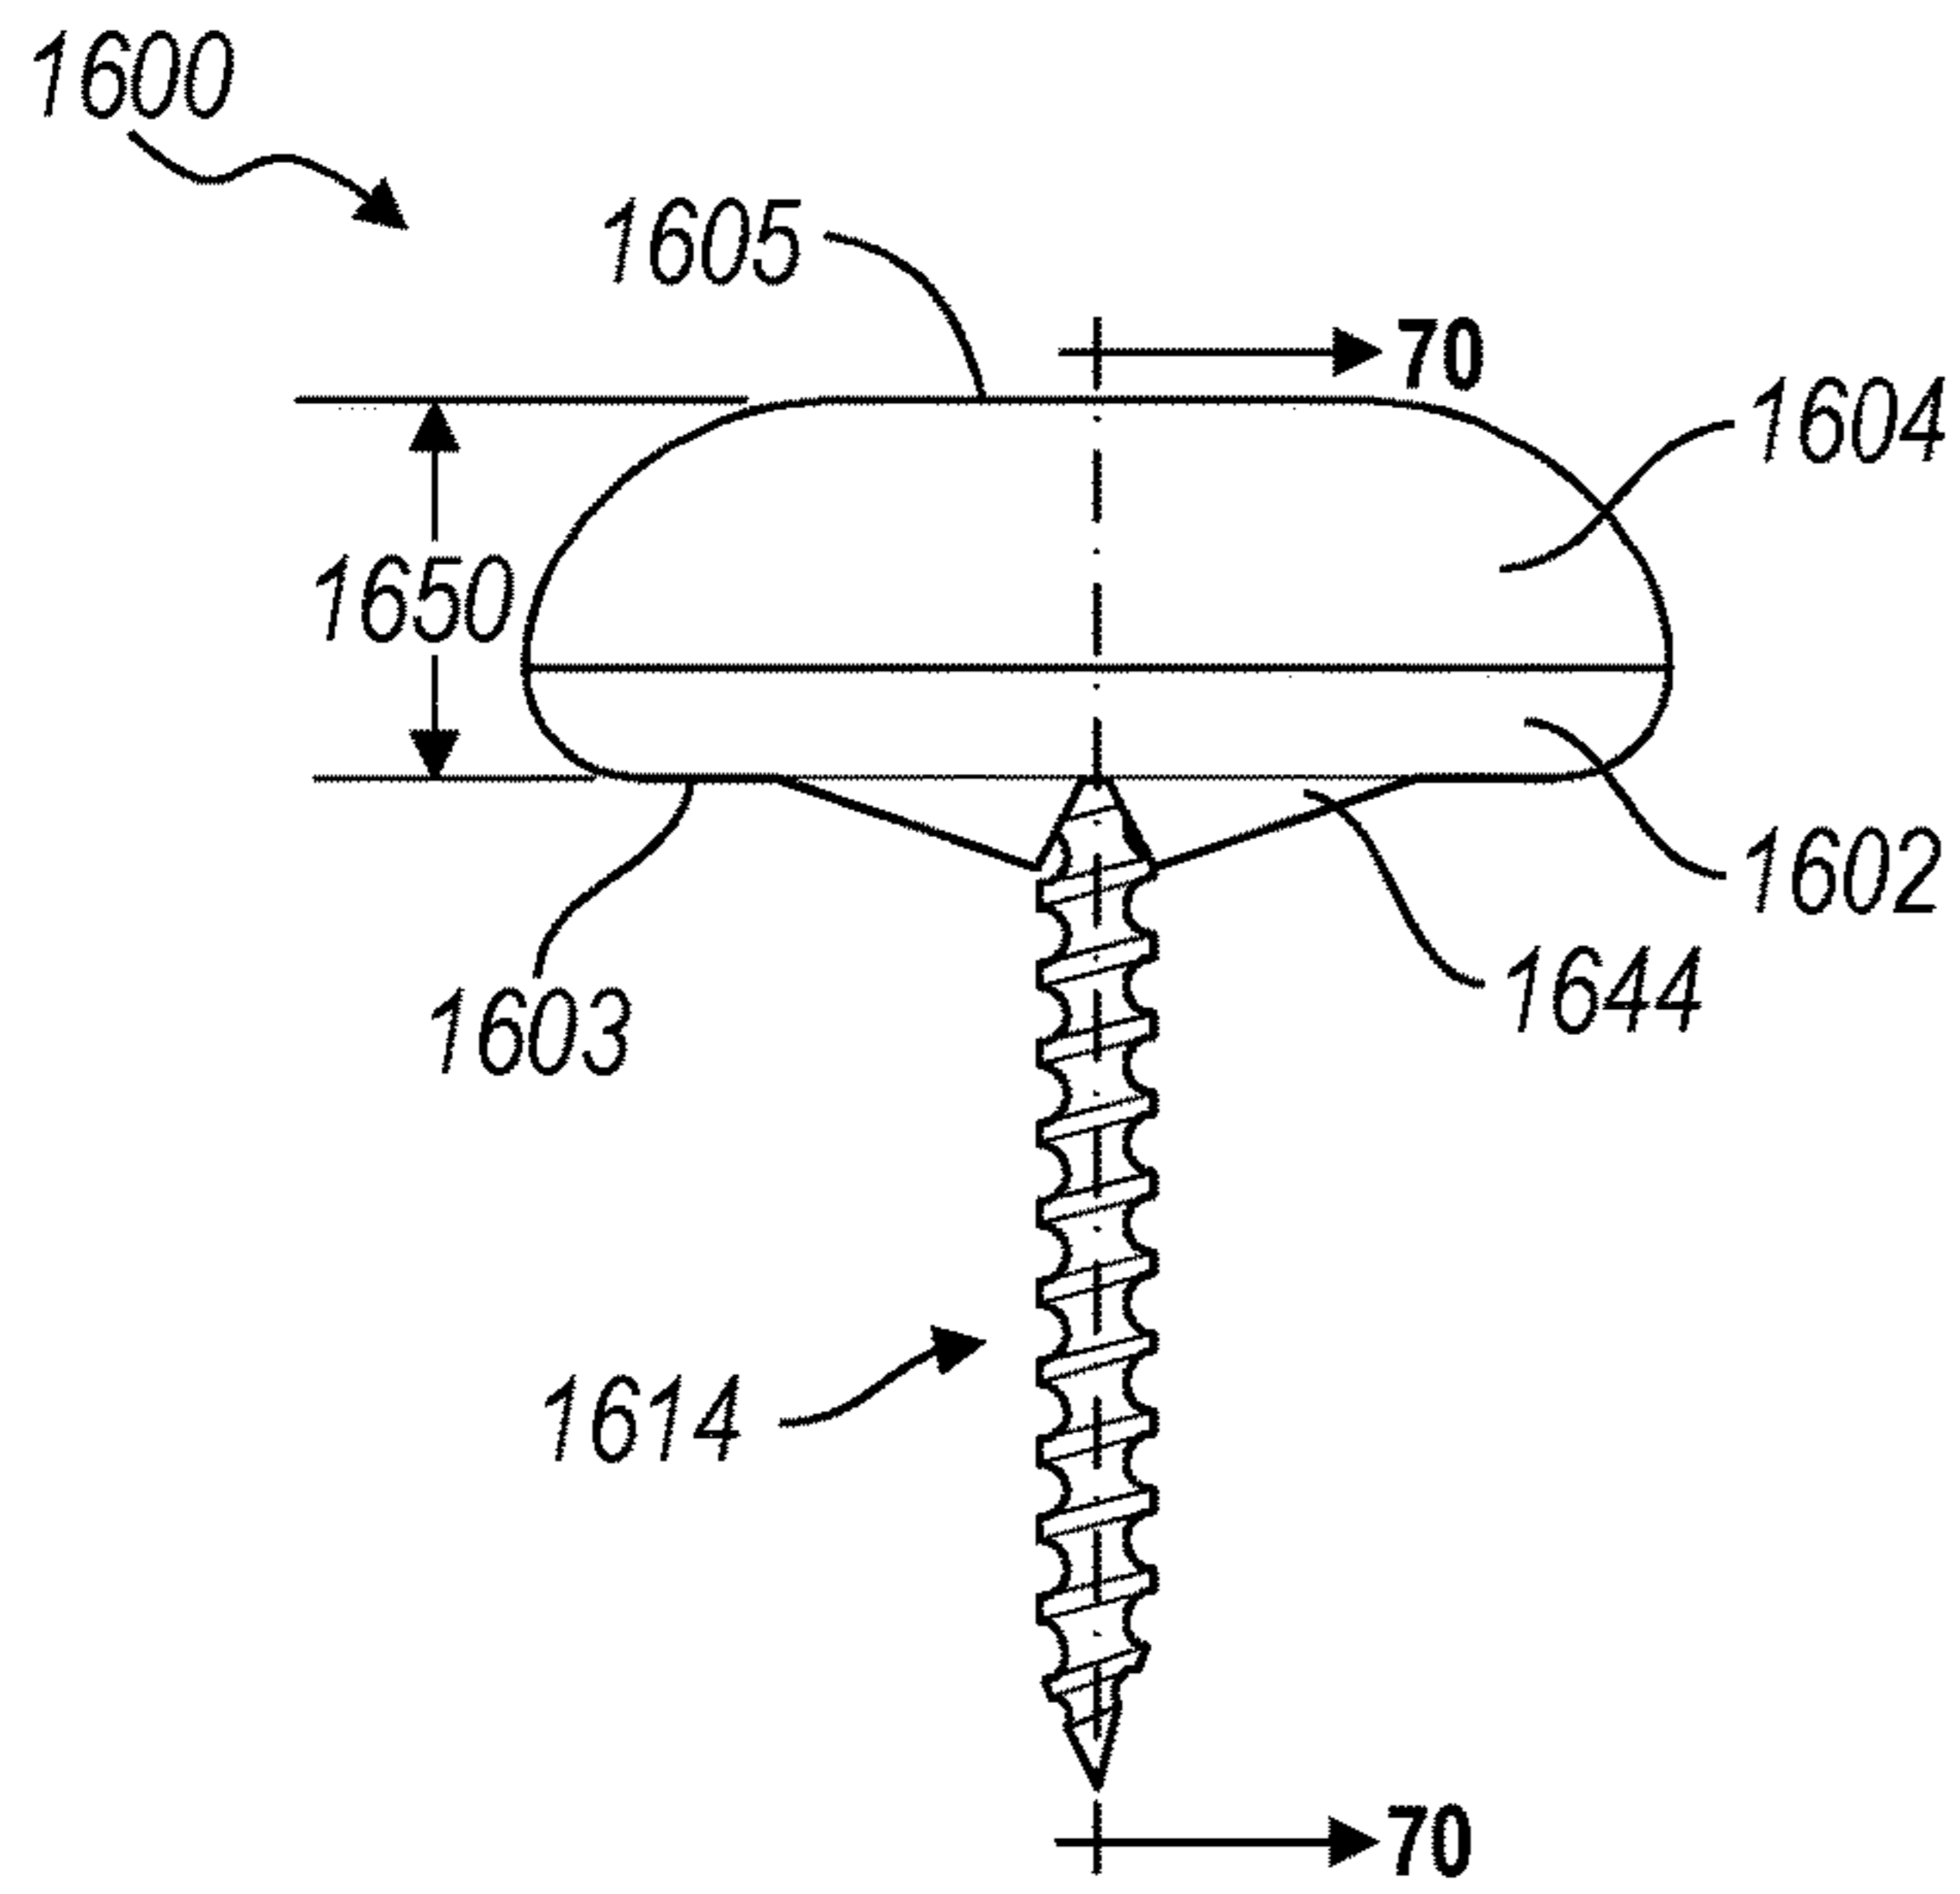


FIG. 69

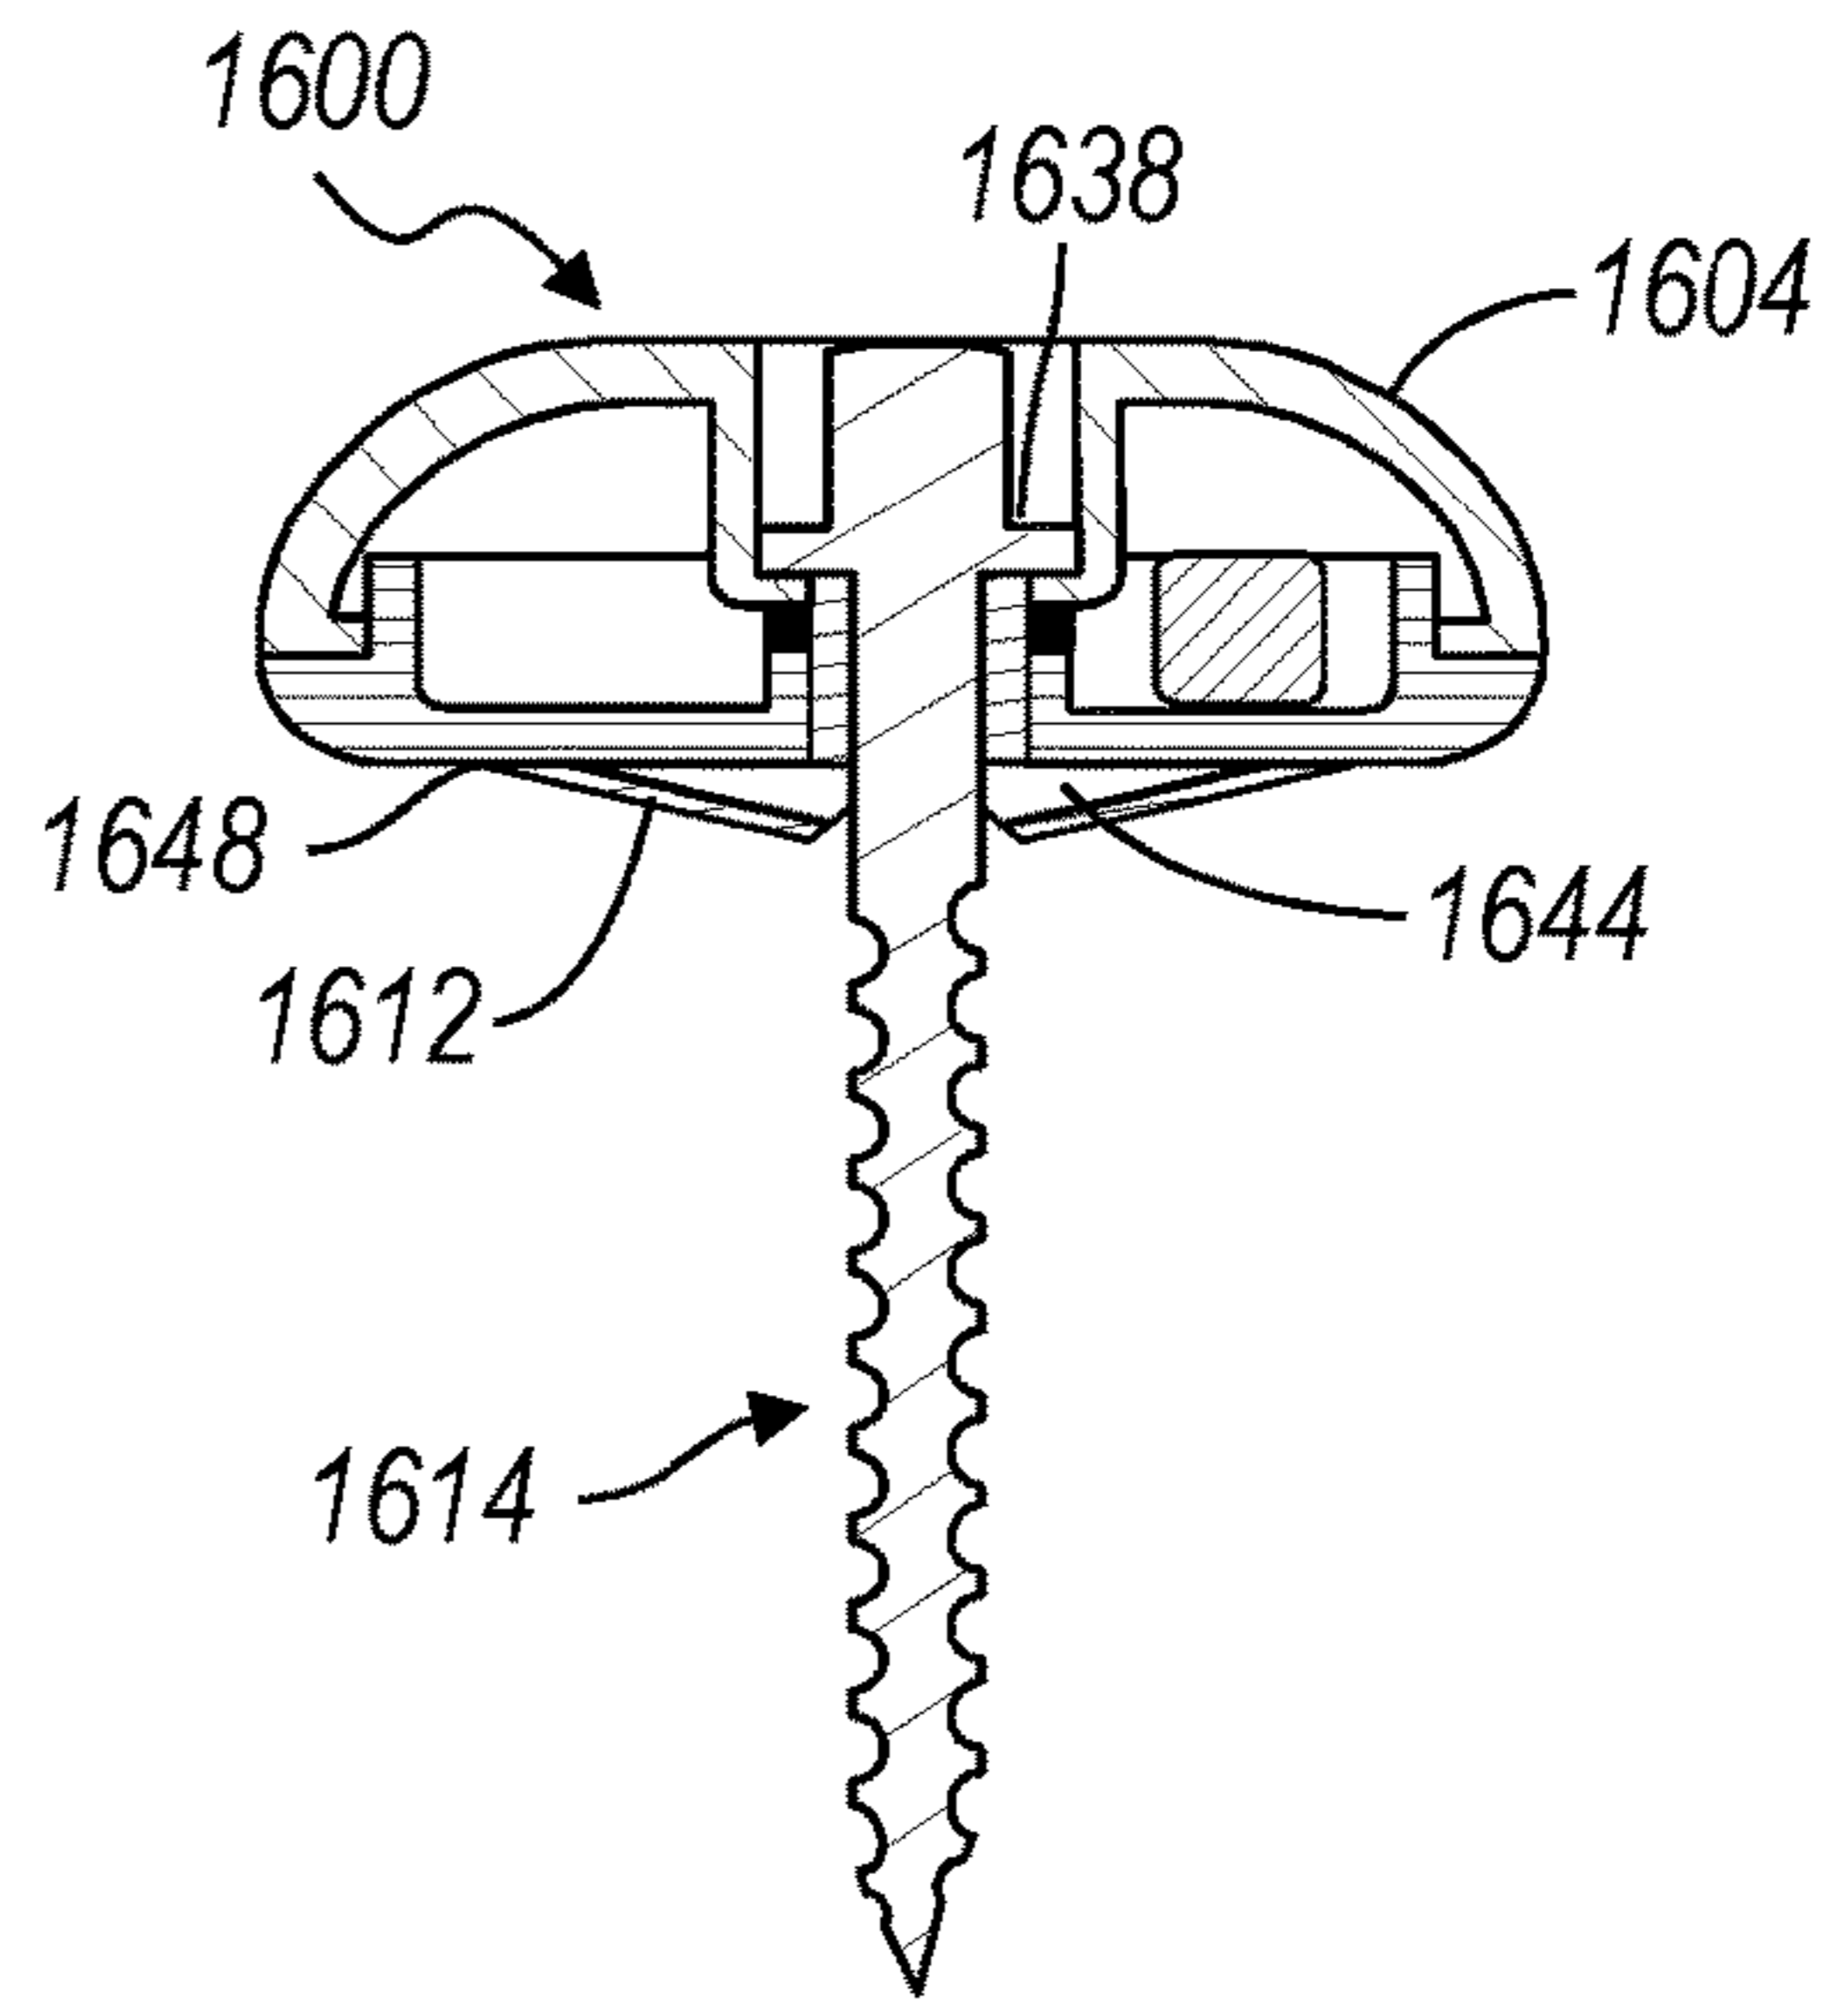


FIG. 70

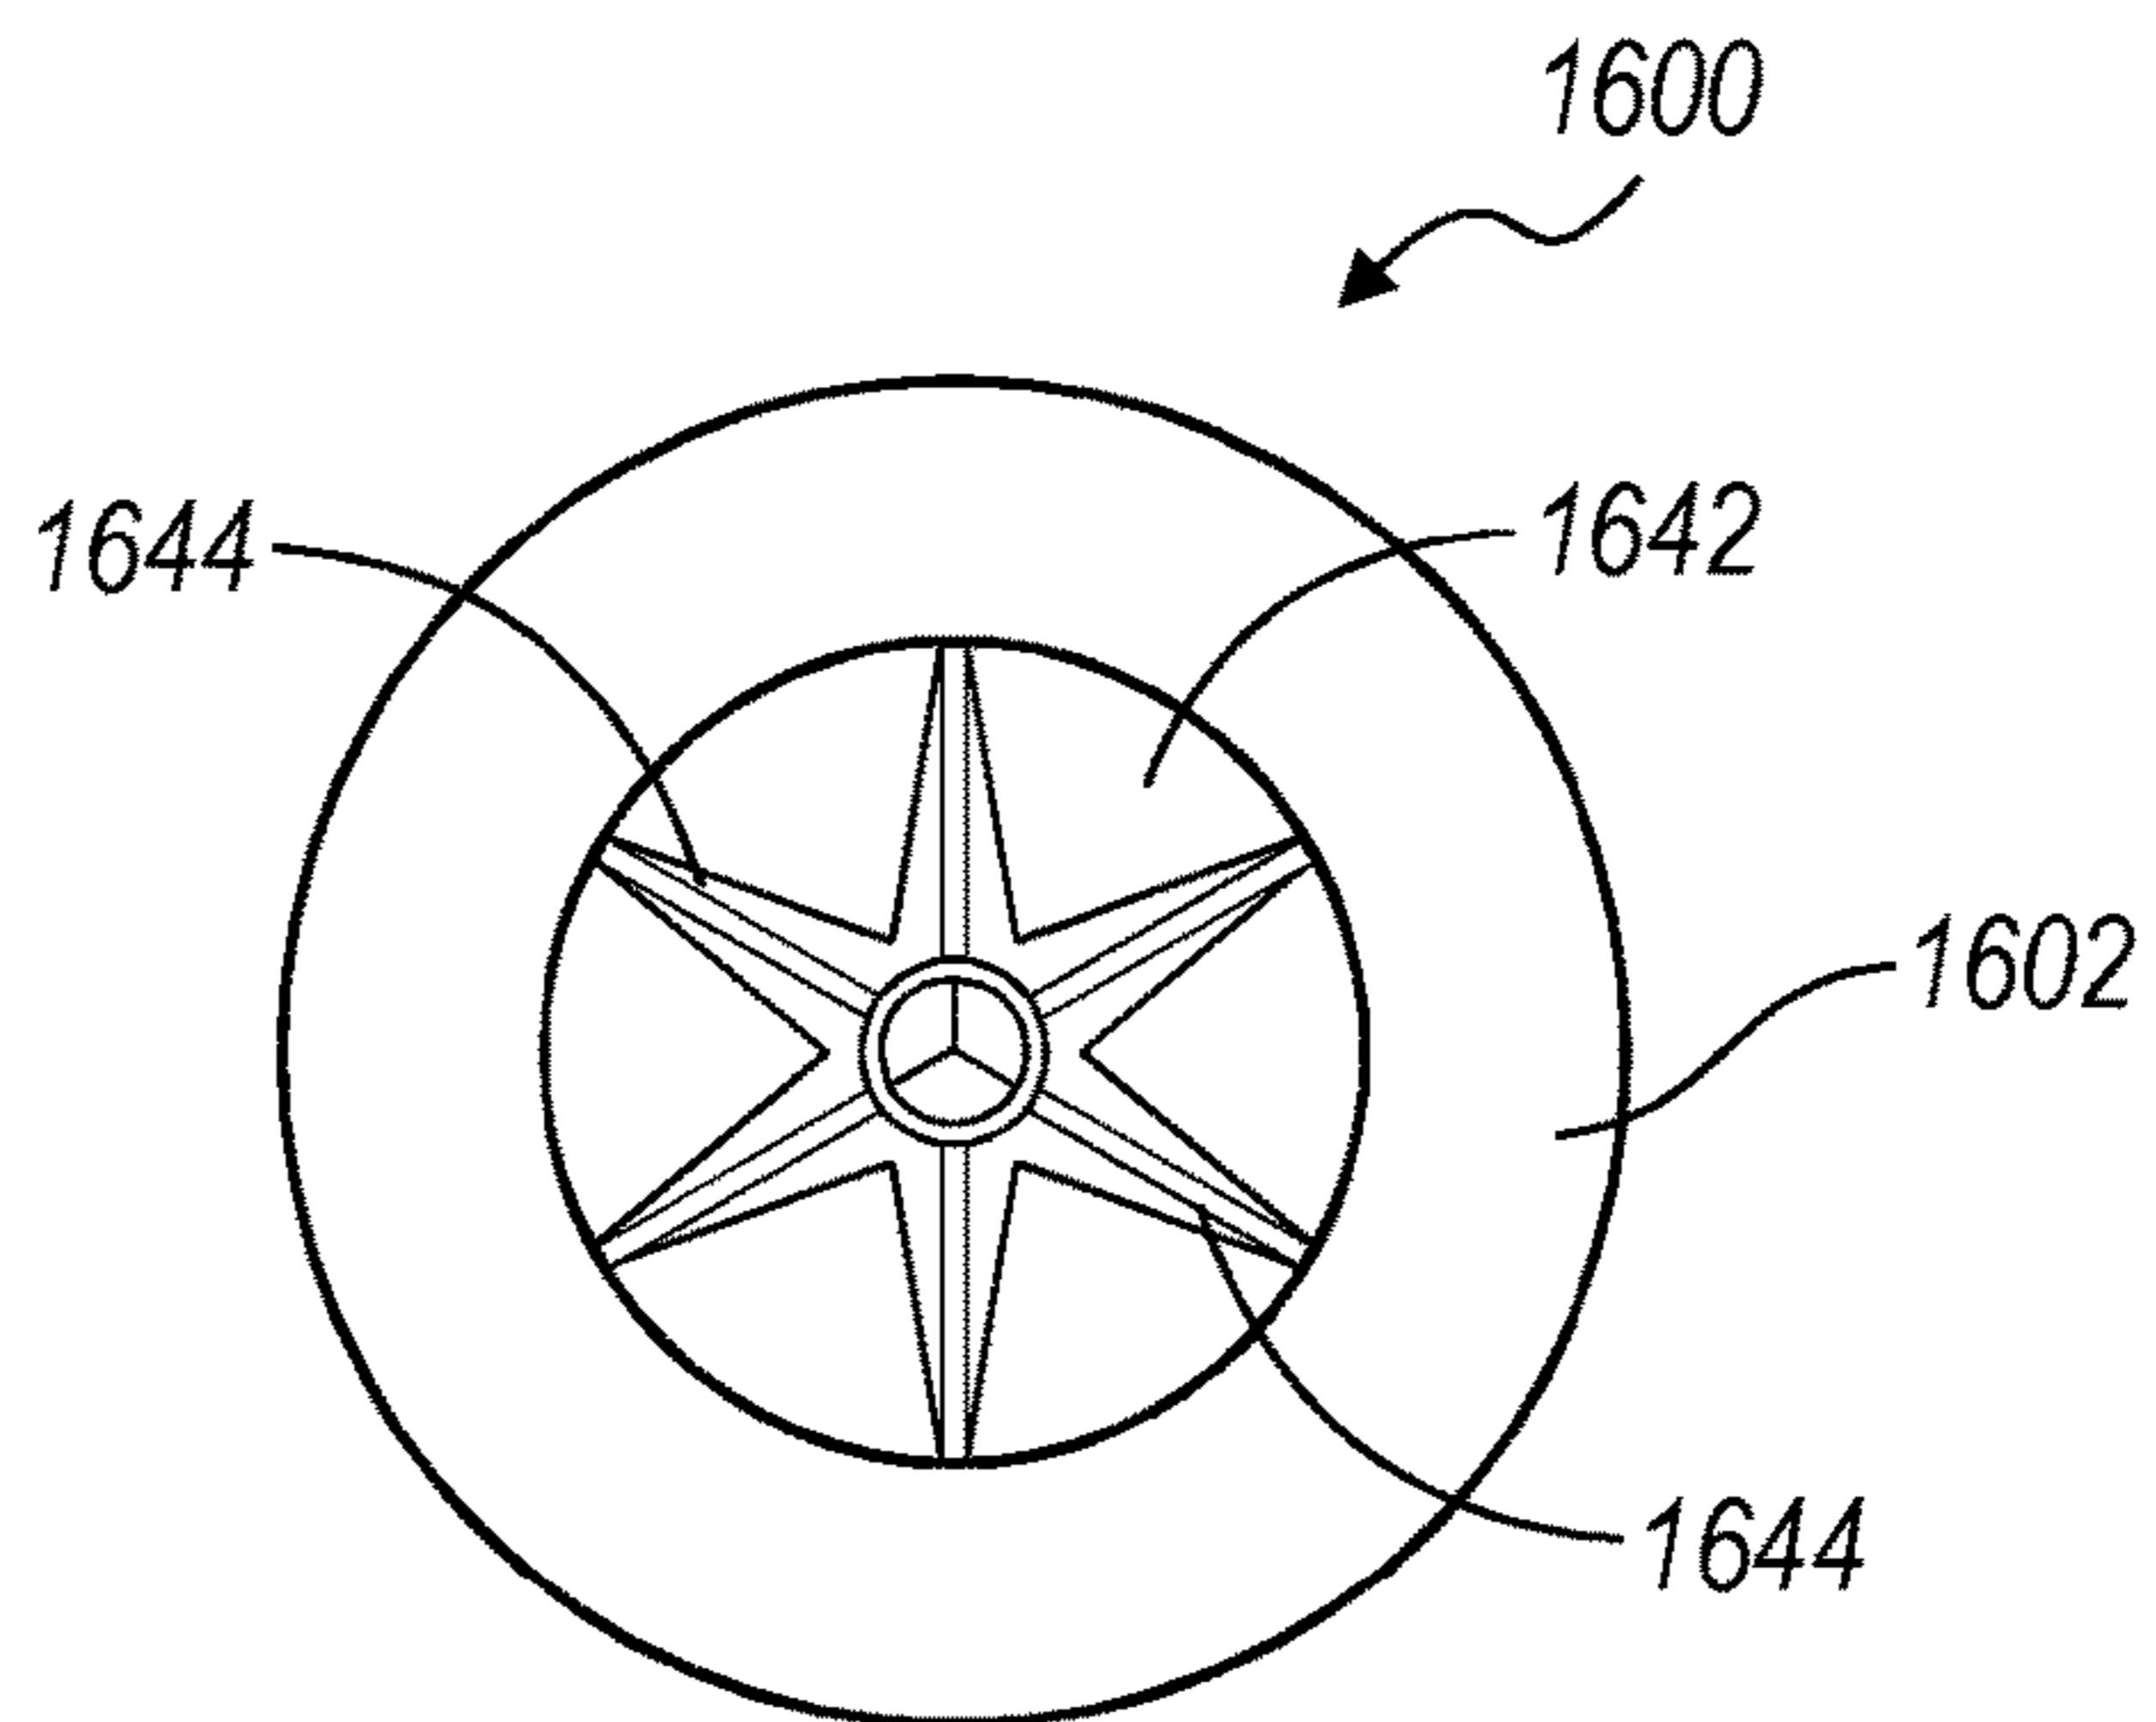


FIG. 71

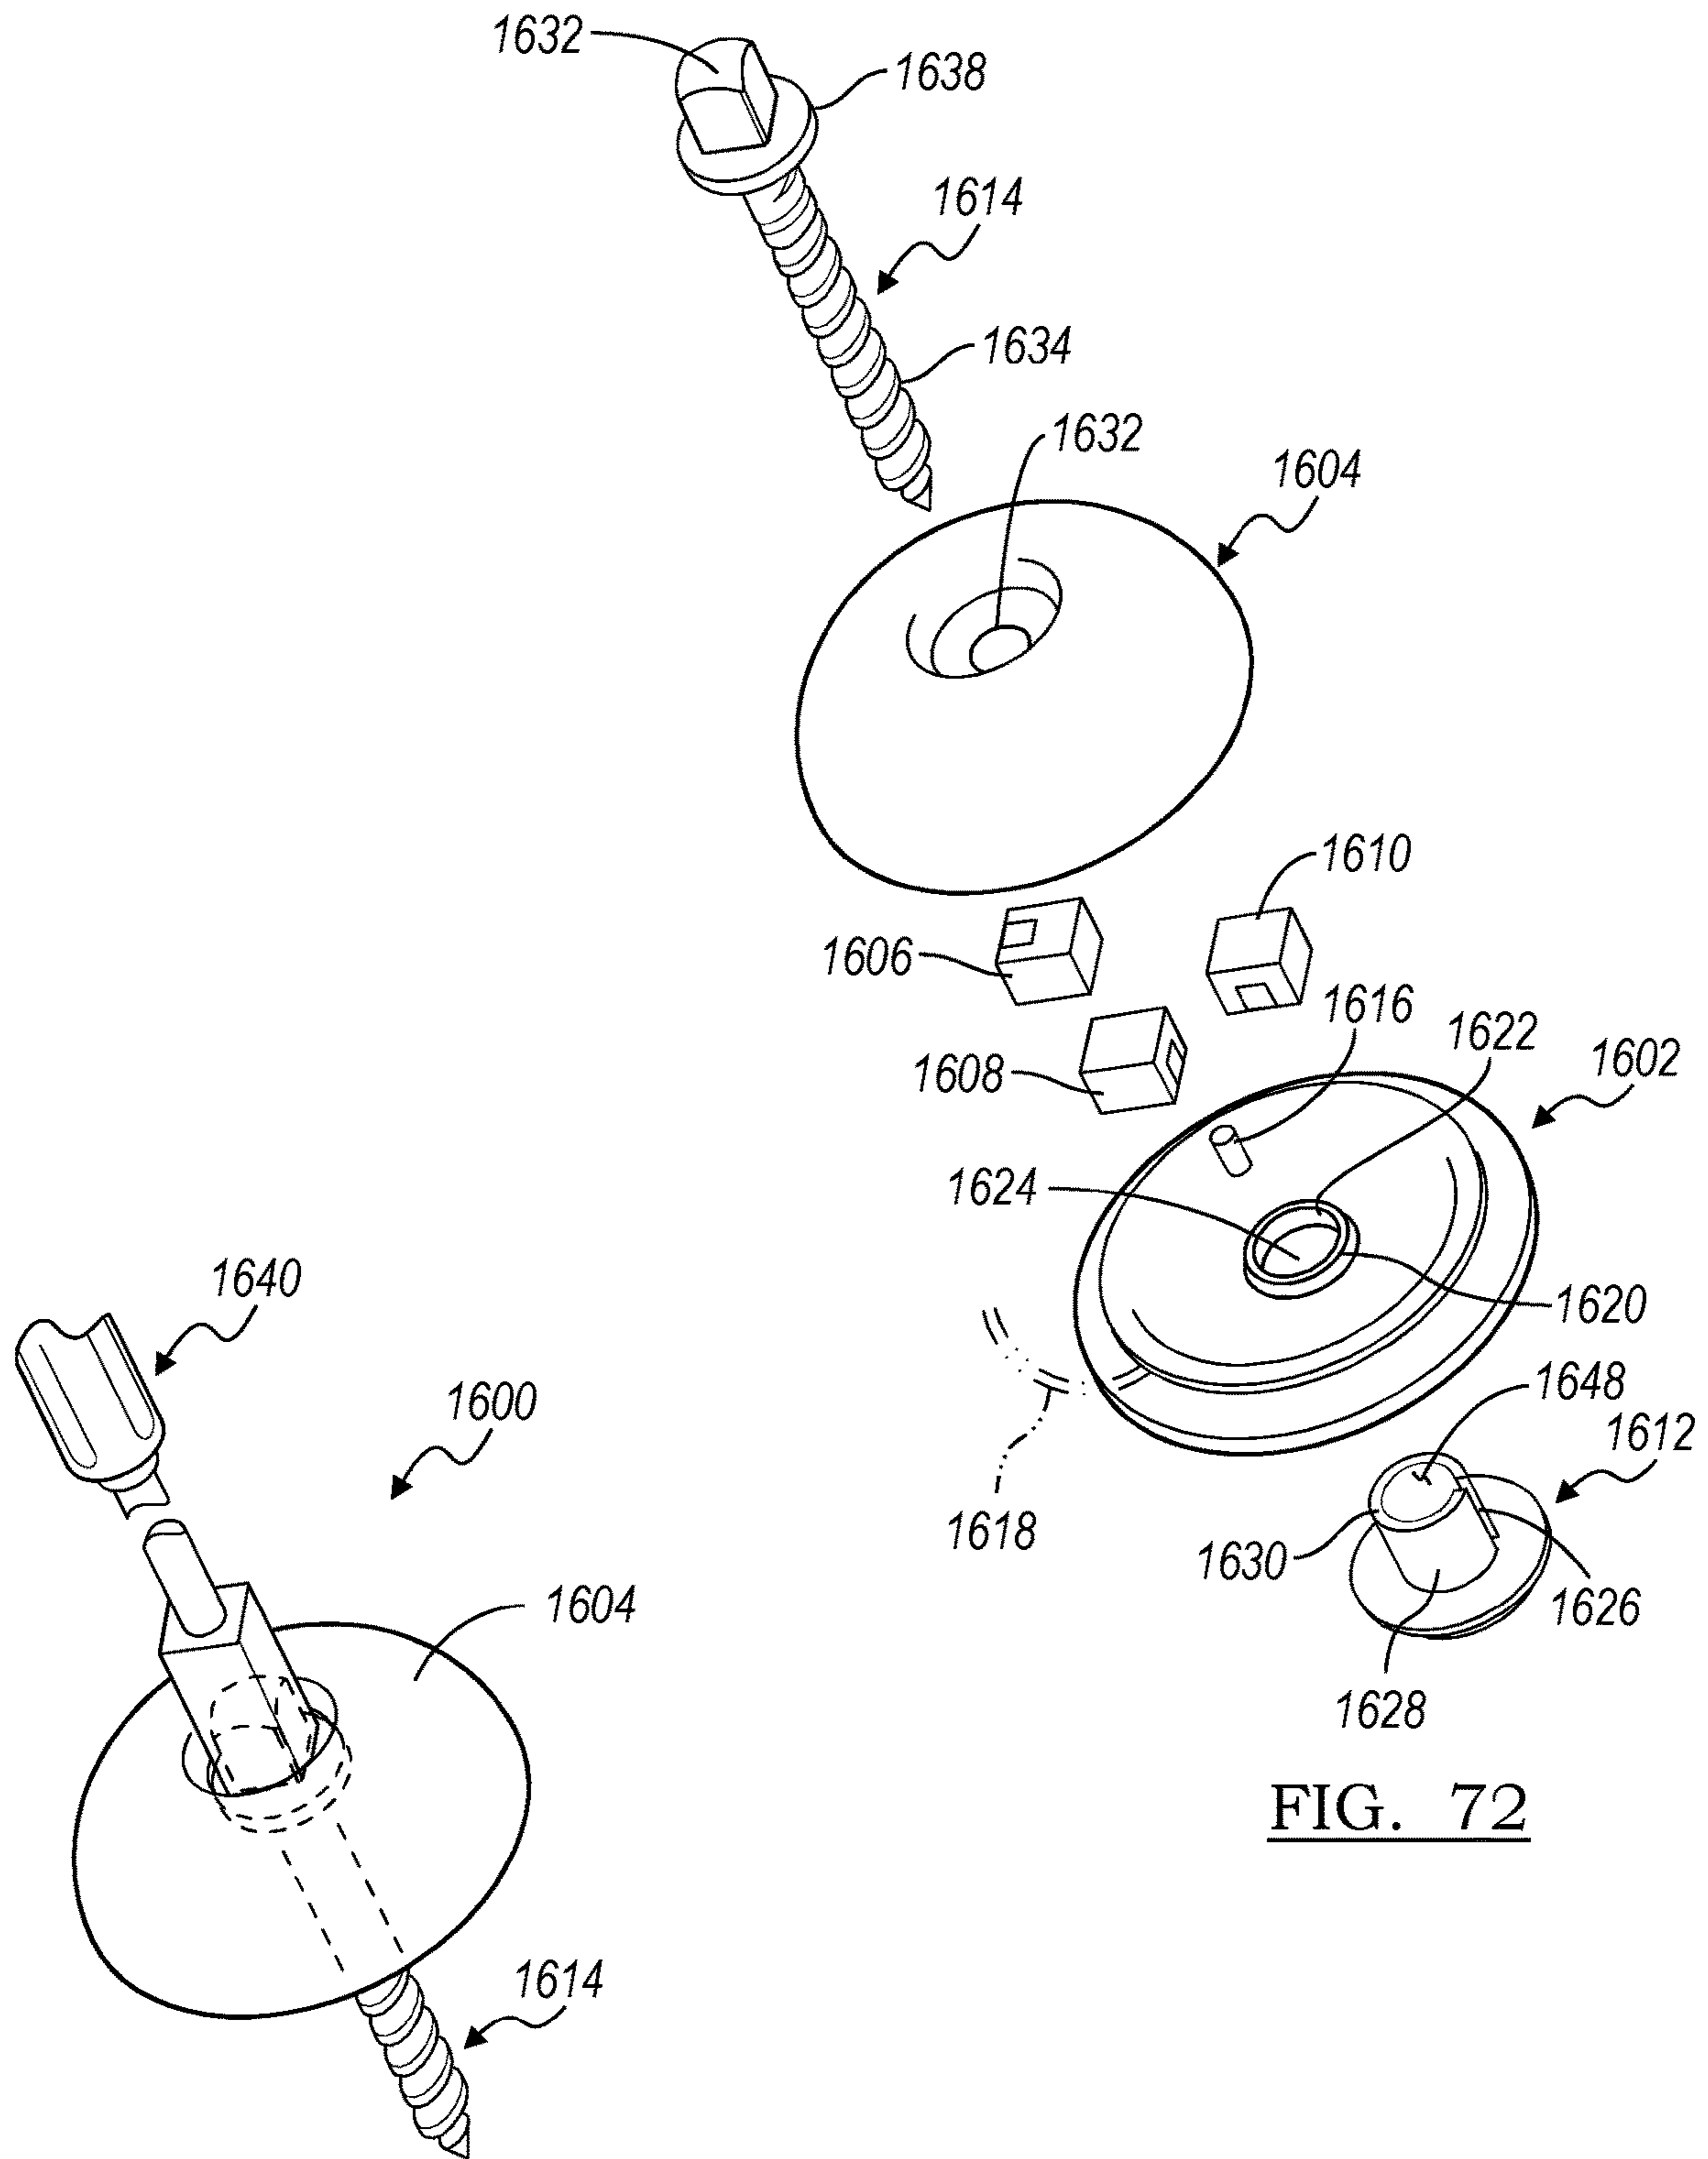


FIG. 72

FIG. 73

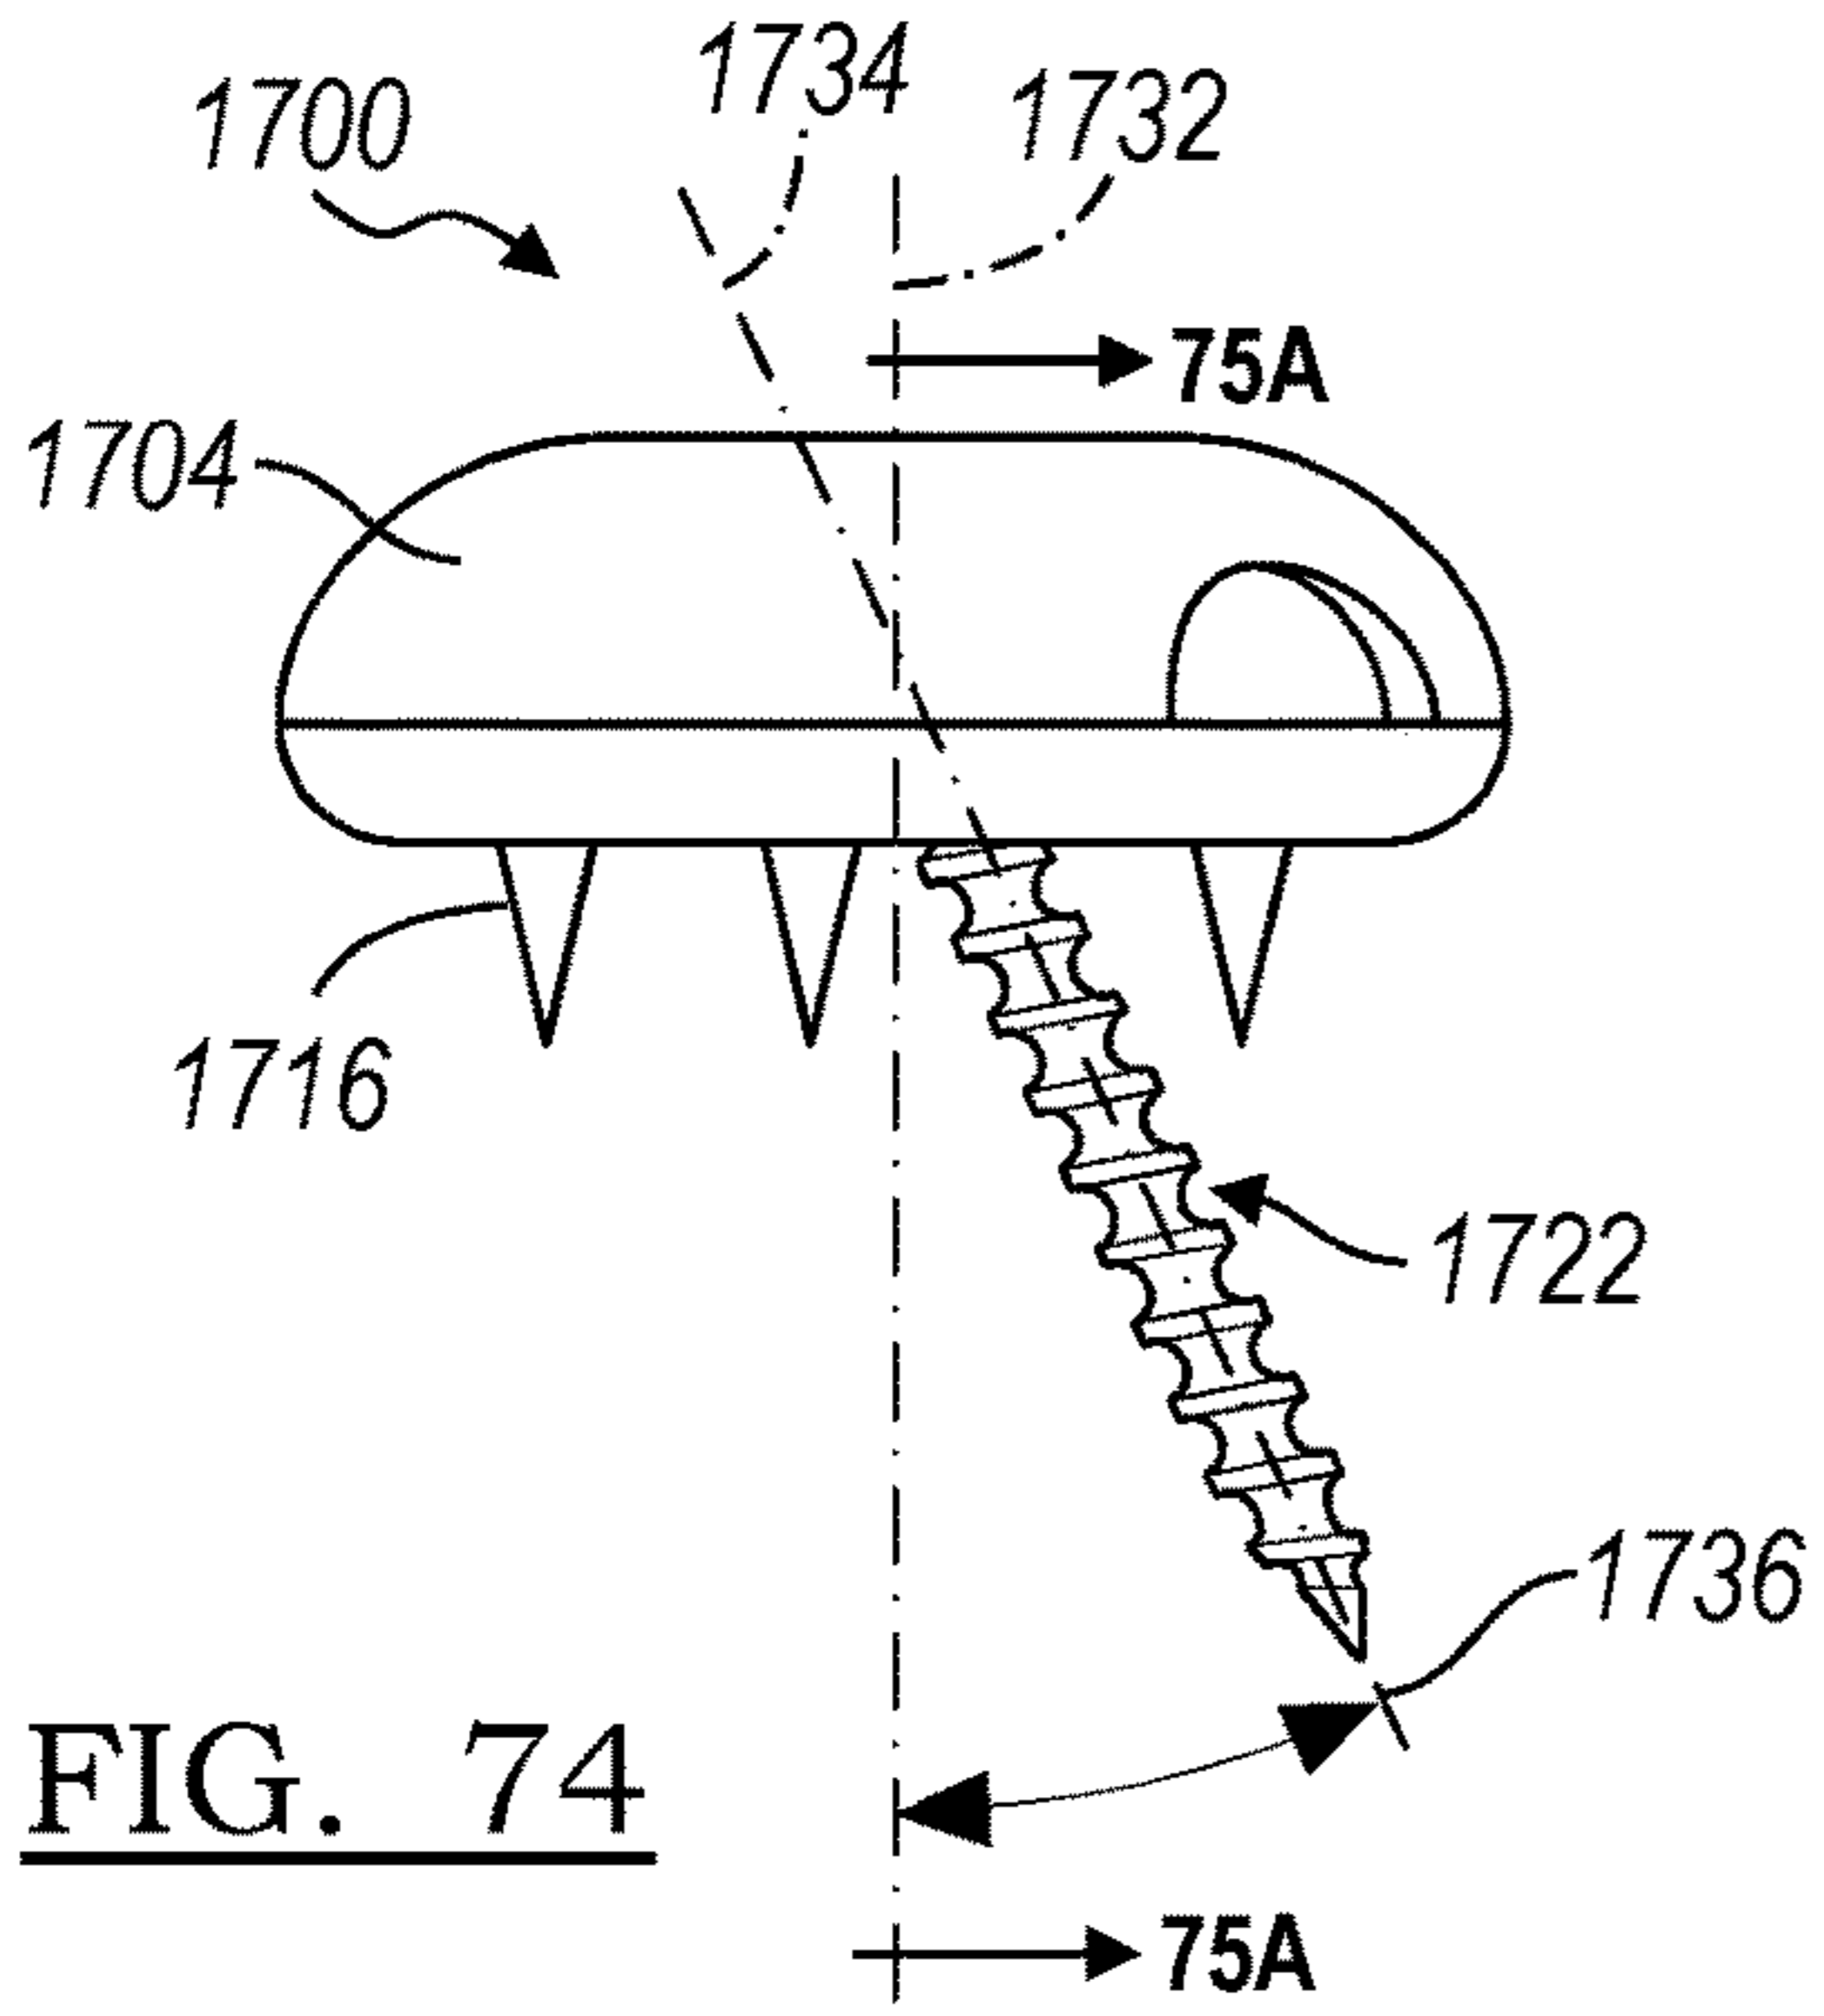


FIG. 74

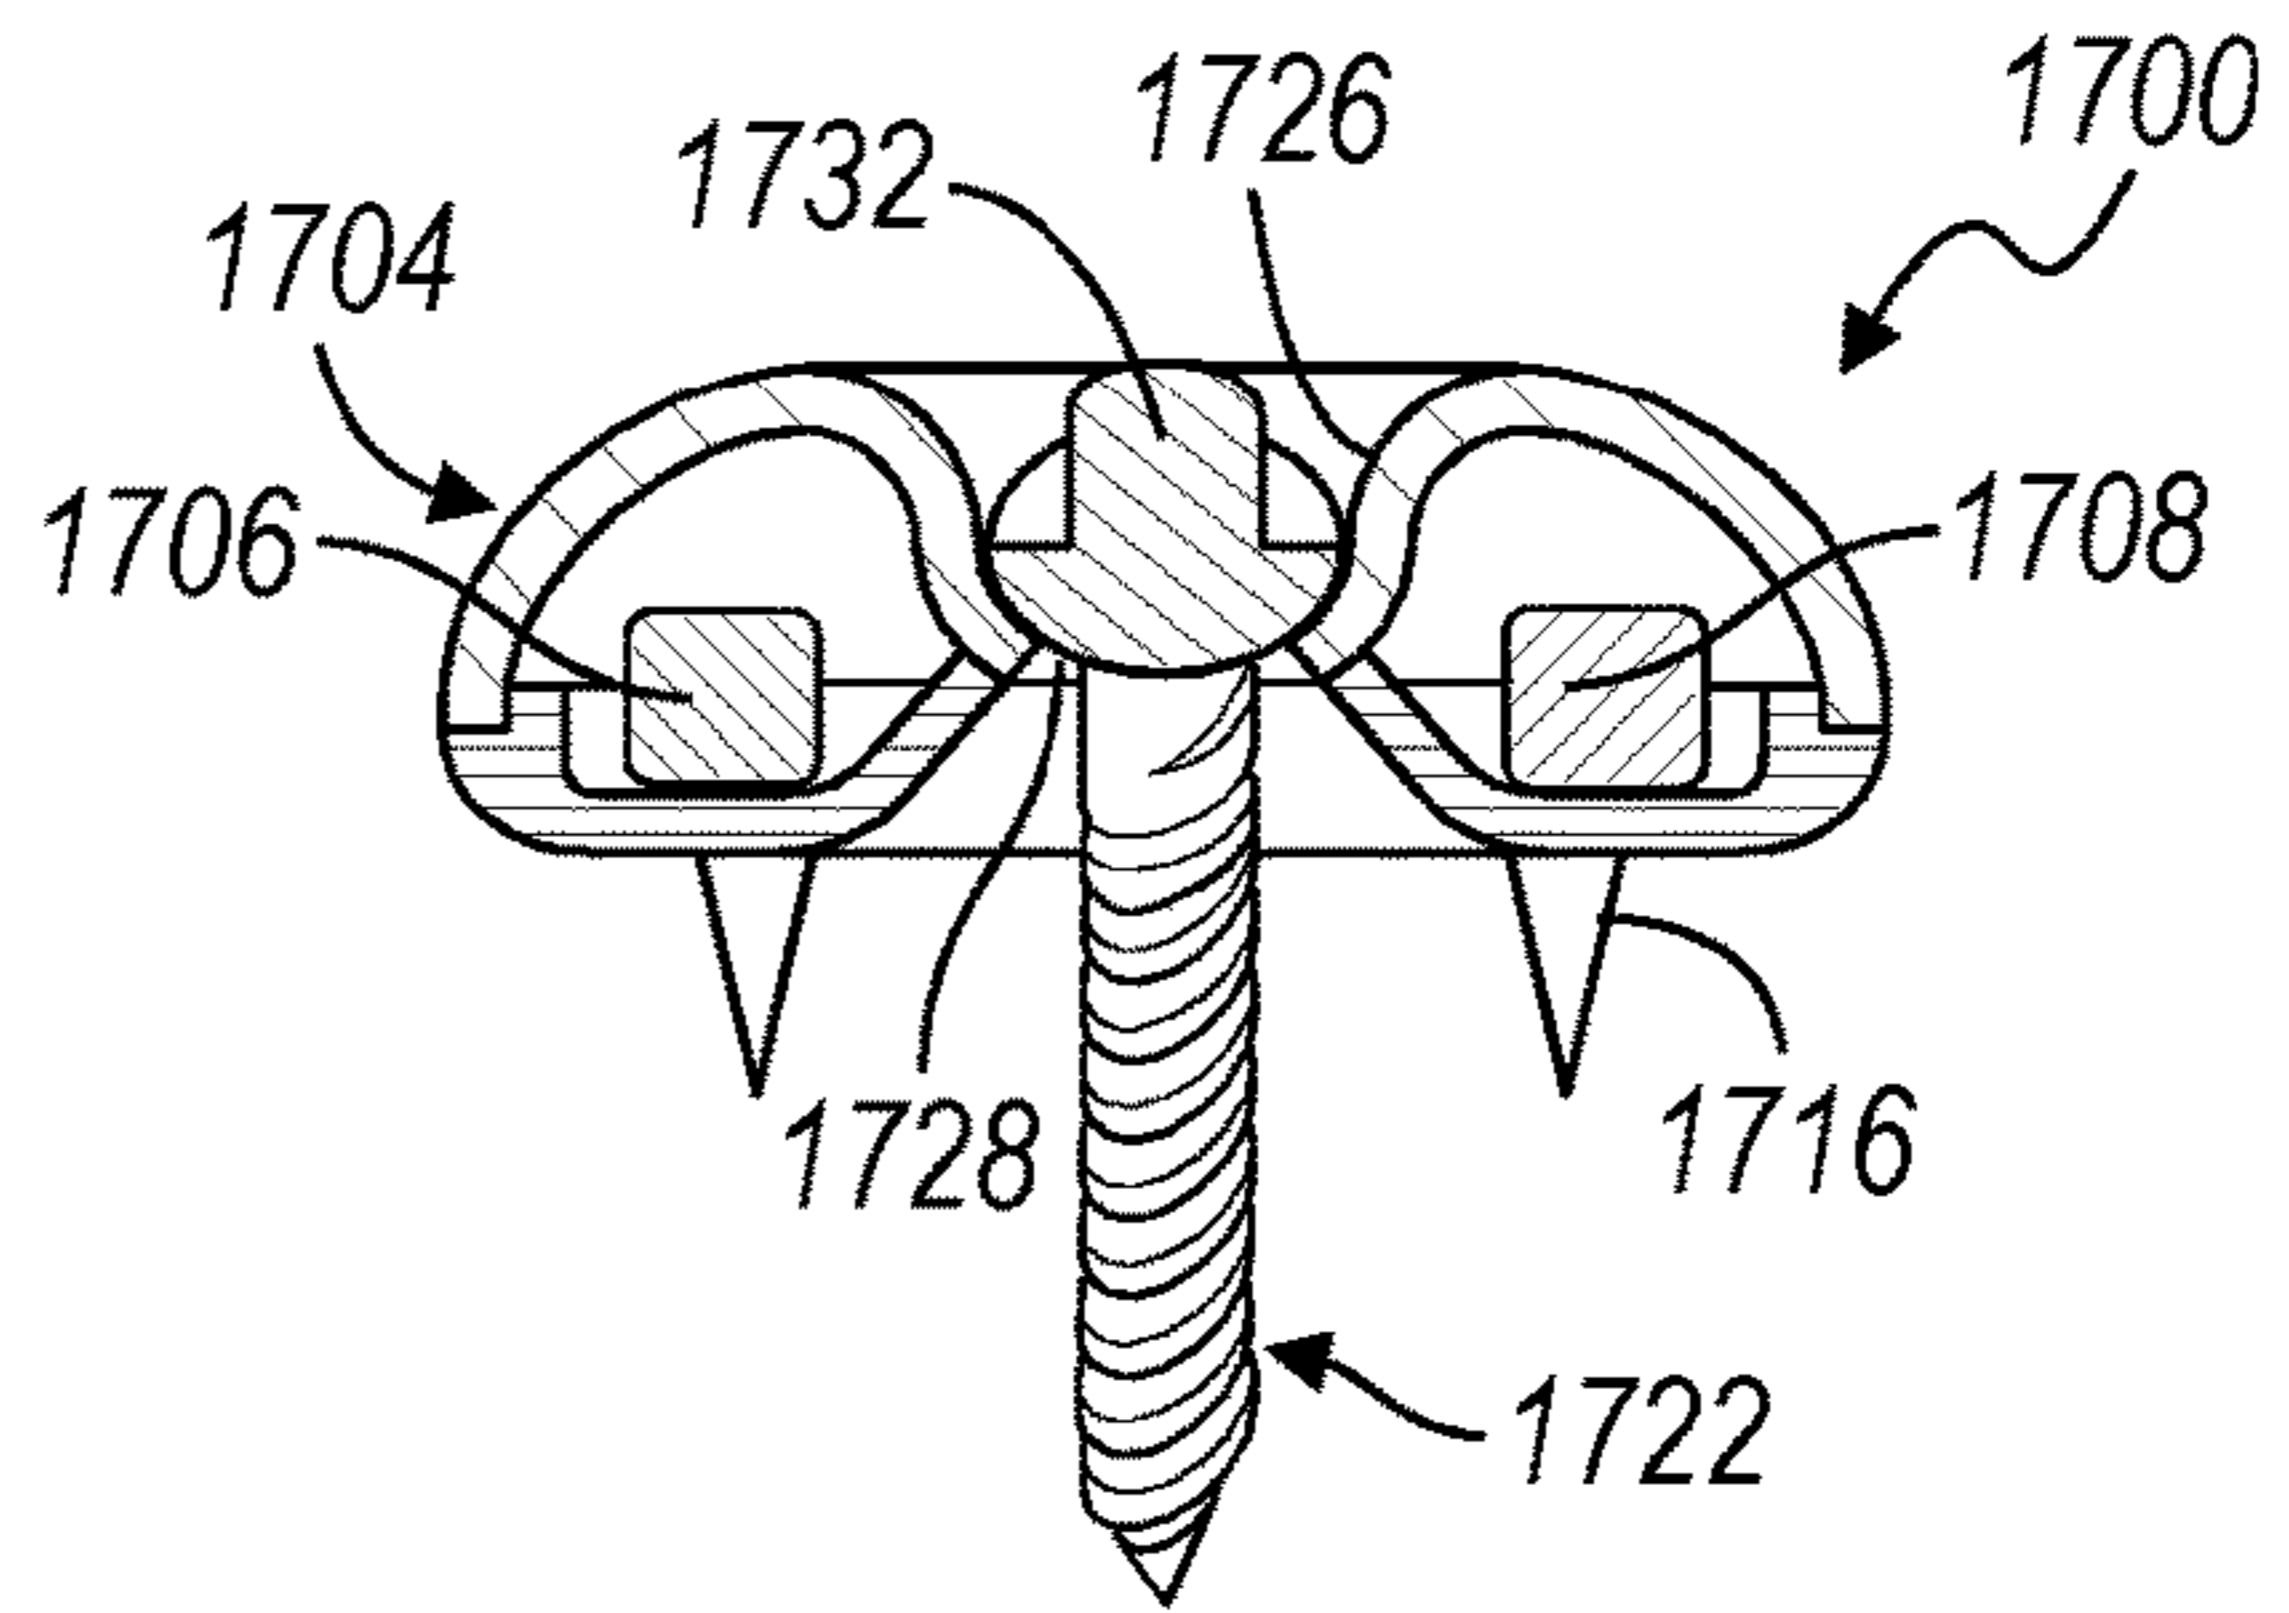


FIG. 75A

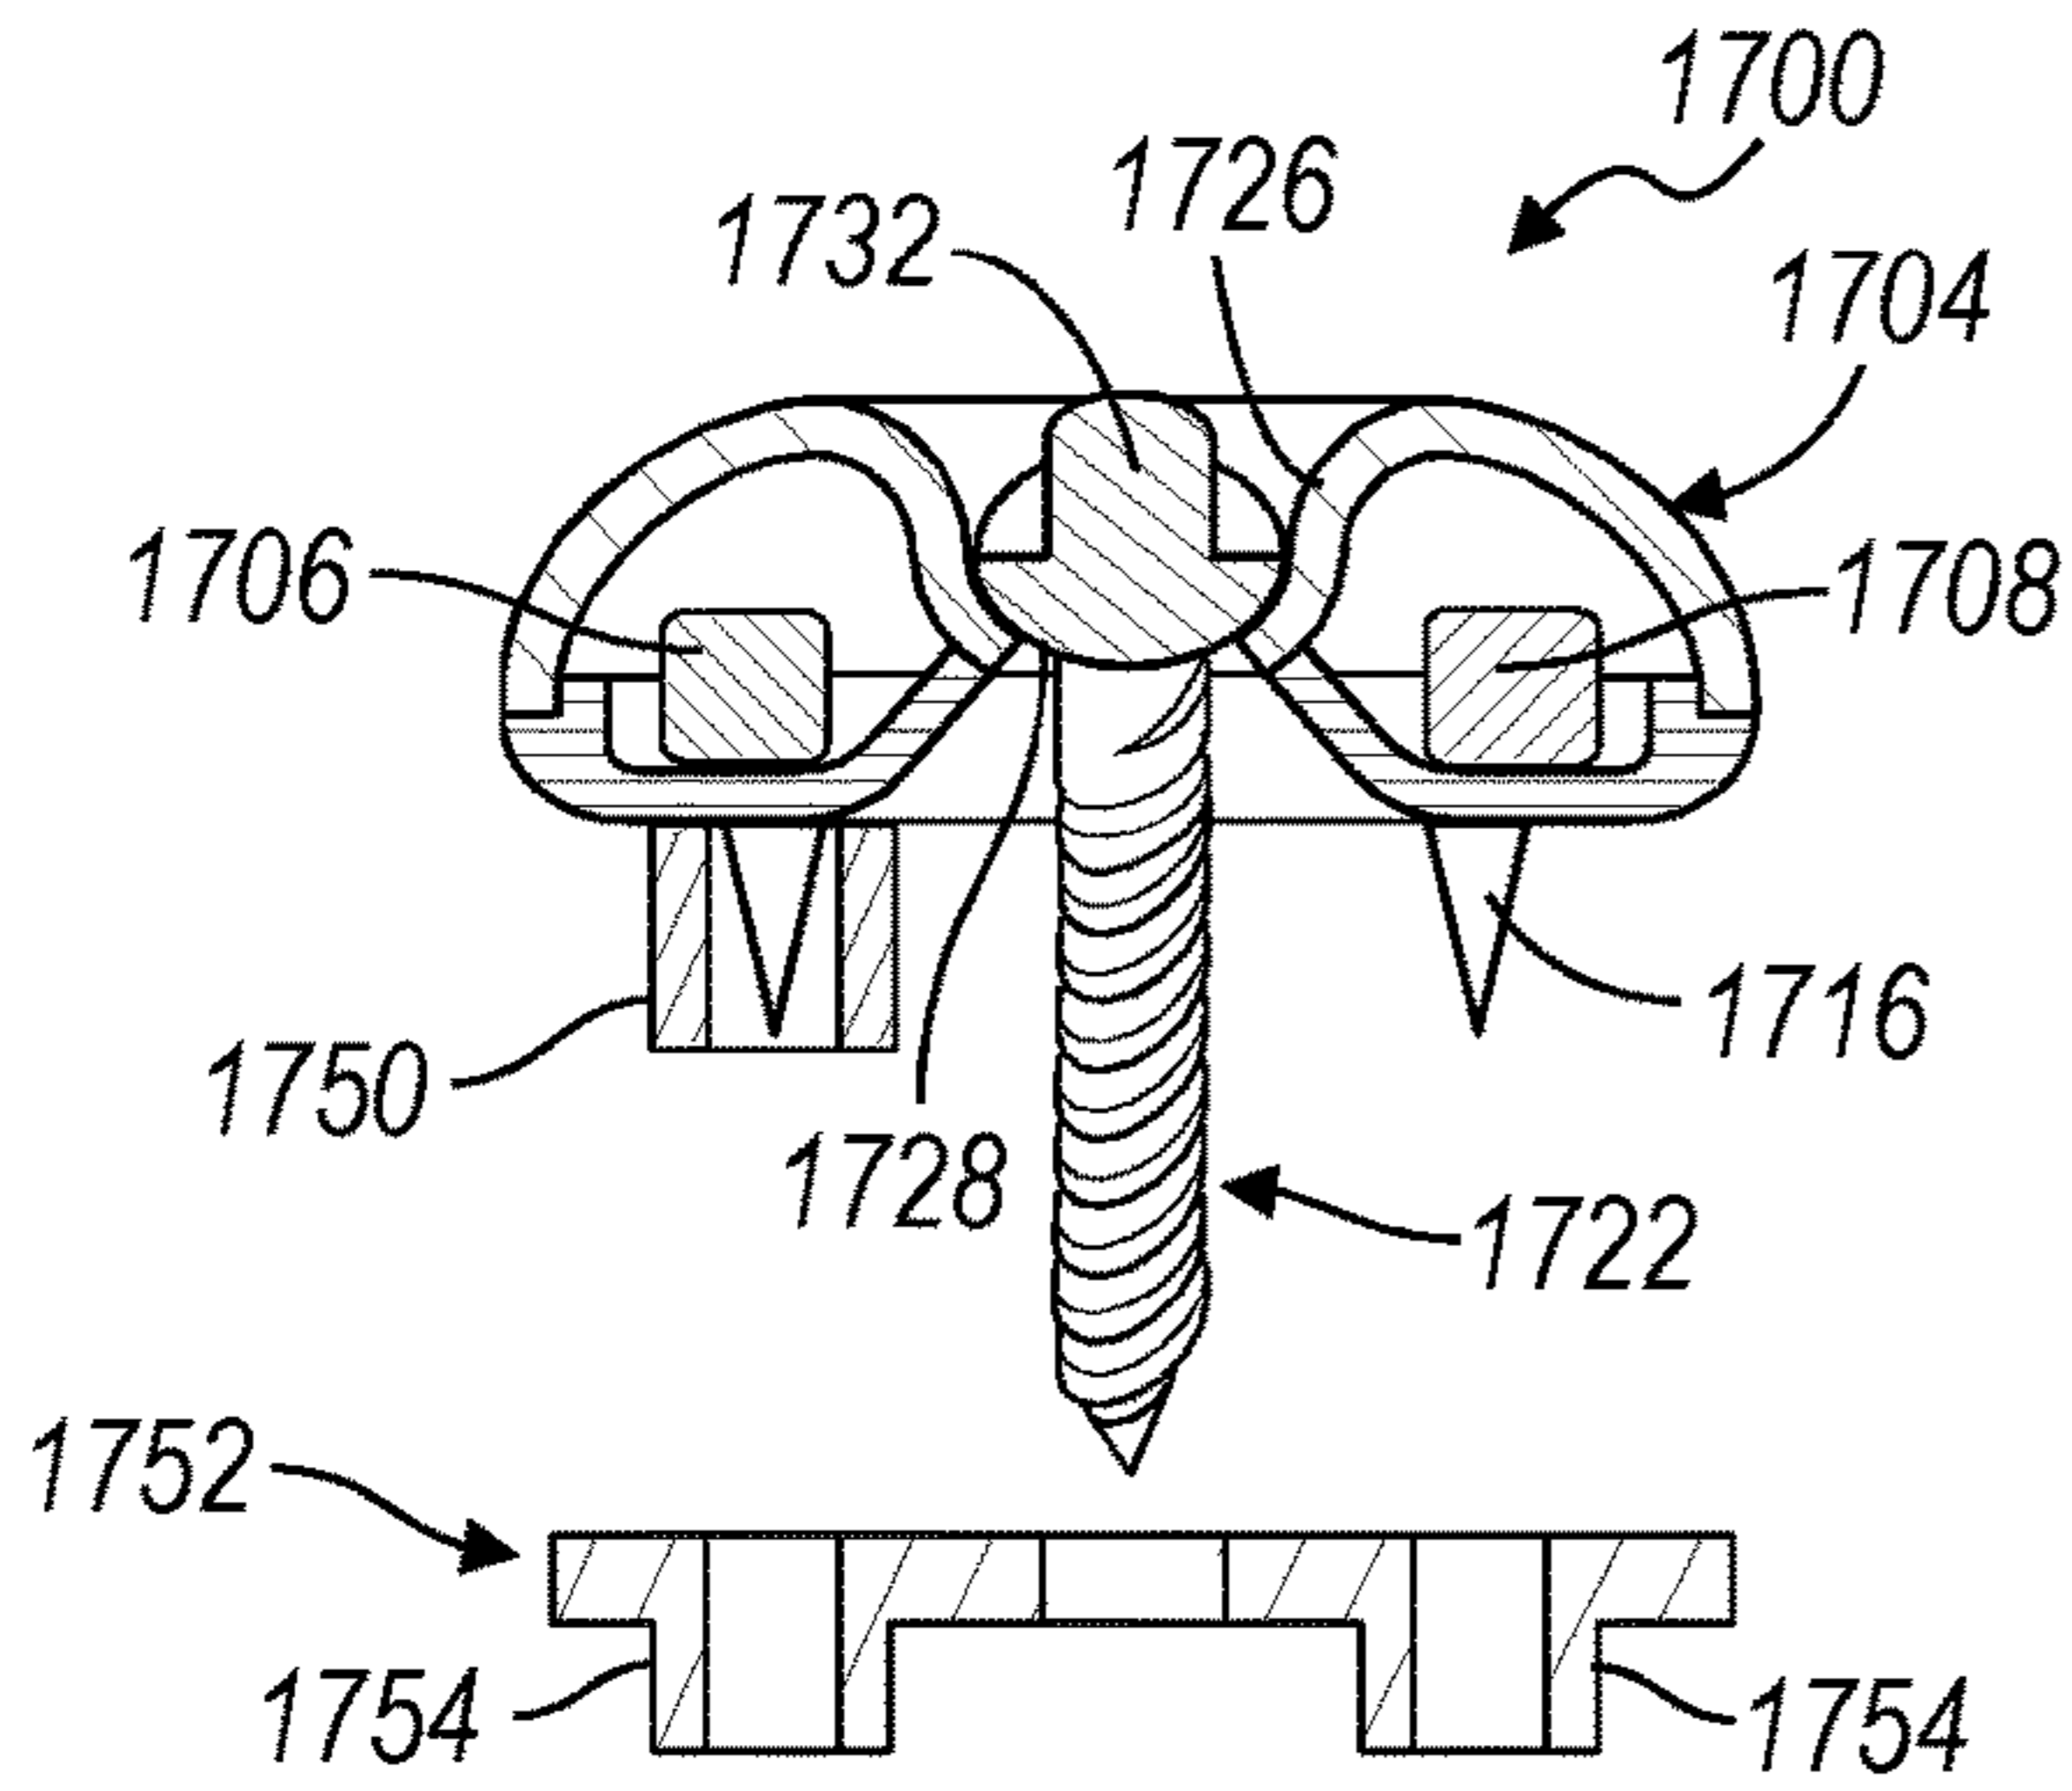


FIG. 75B

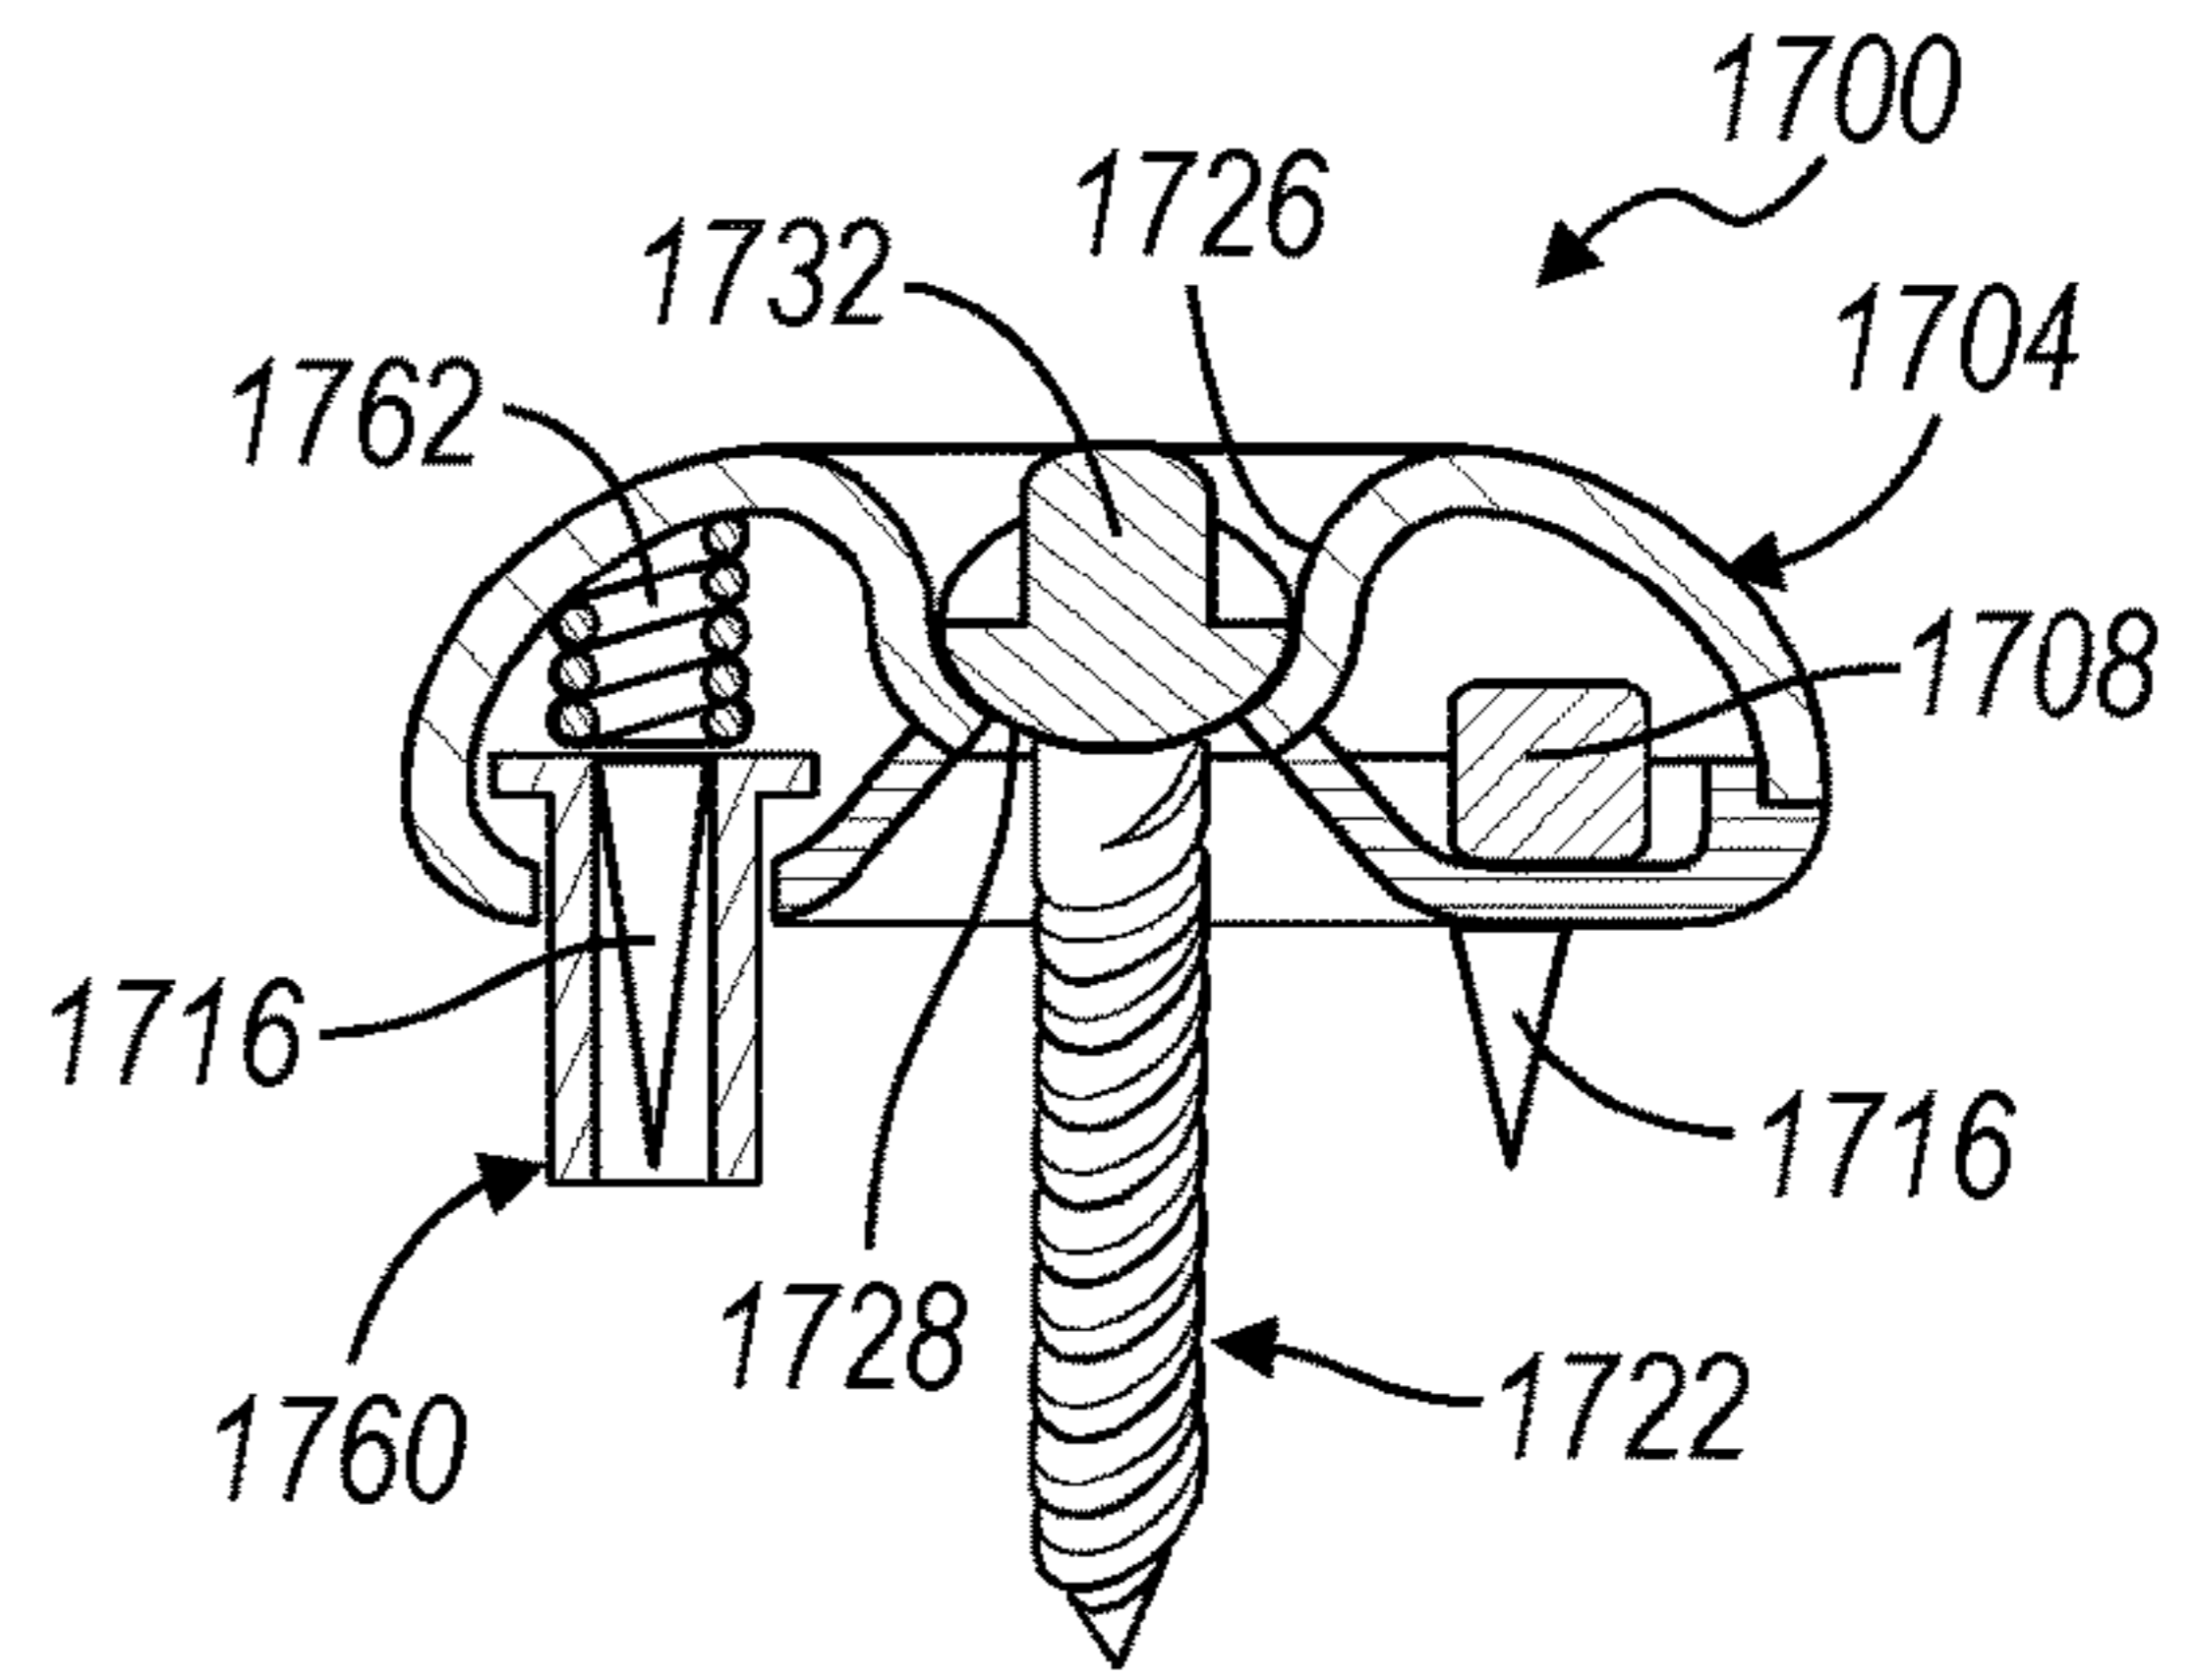


FIG. 75C

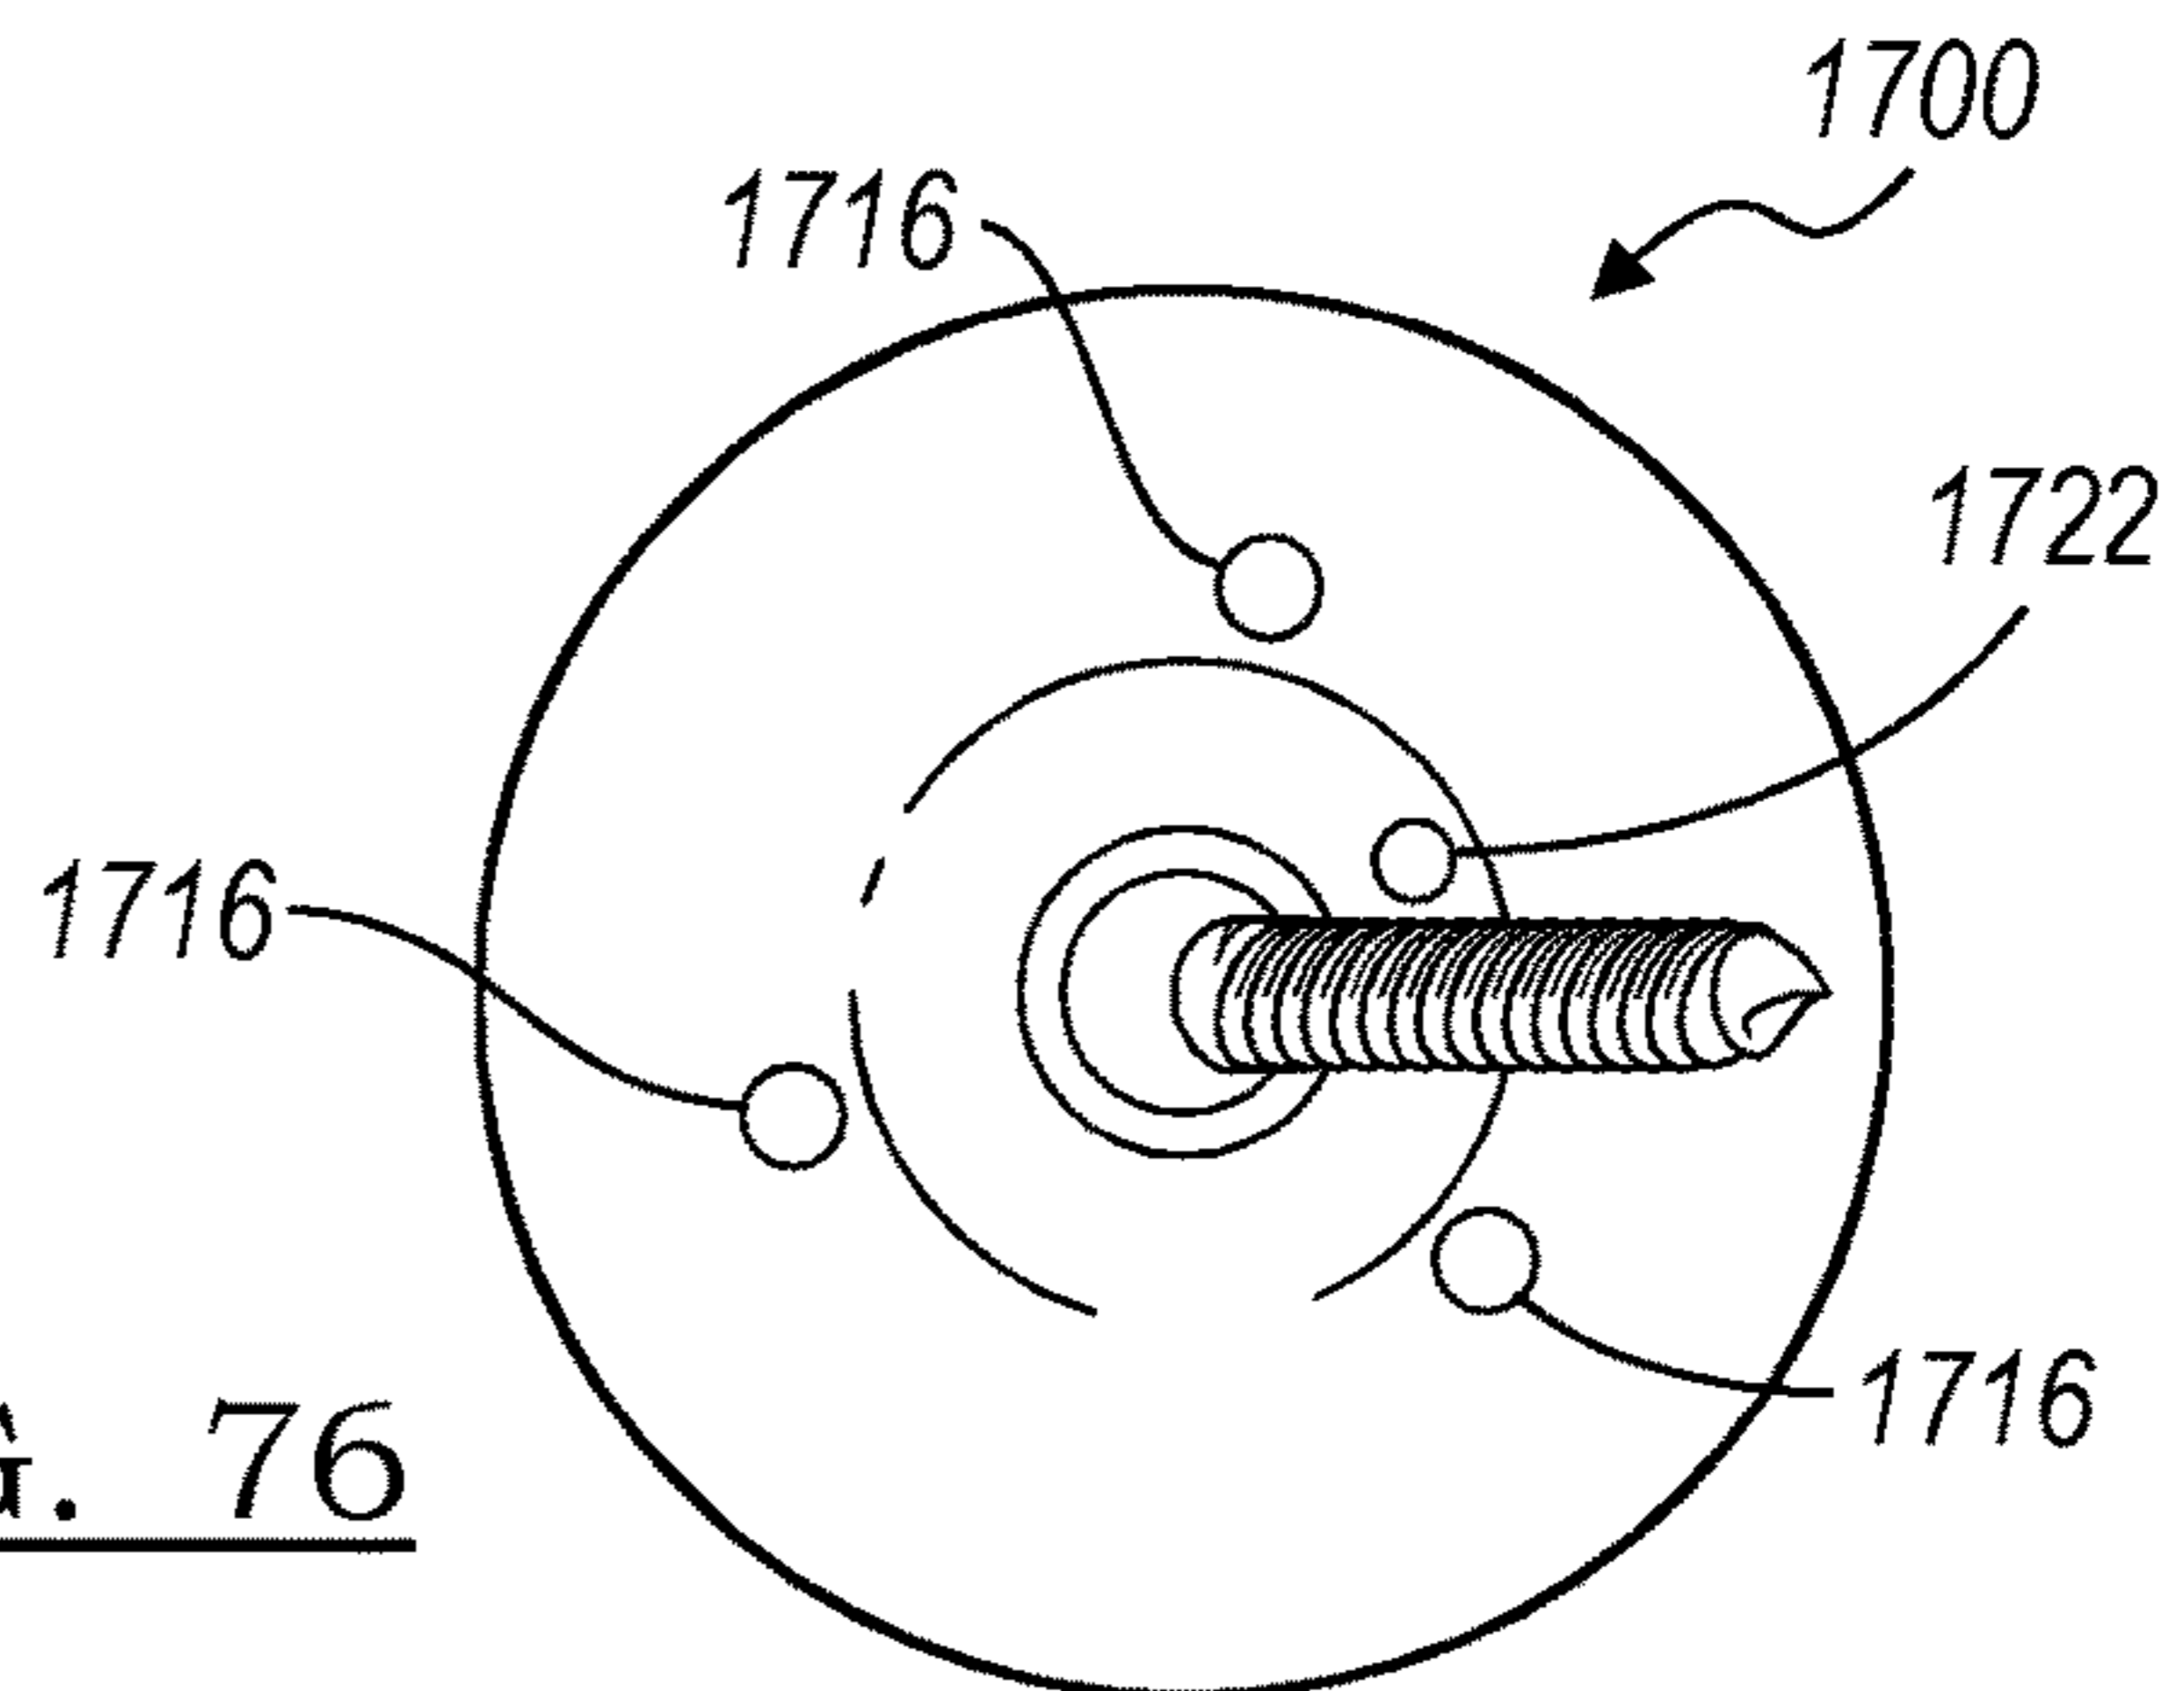


FIG. 76

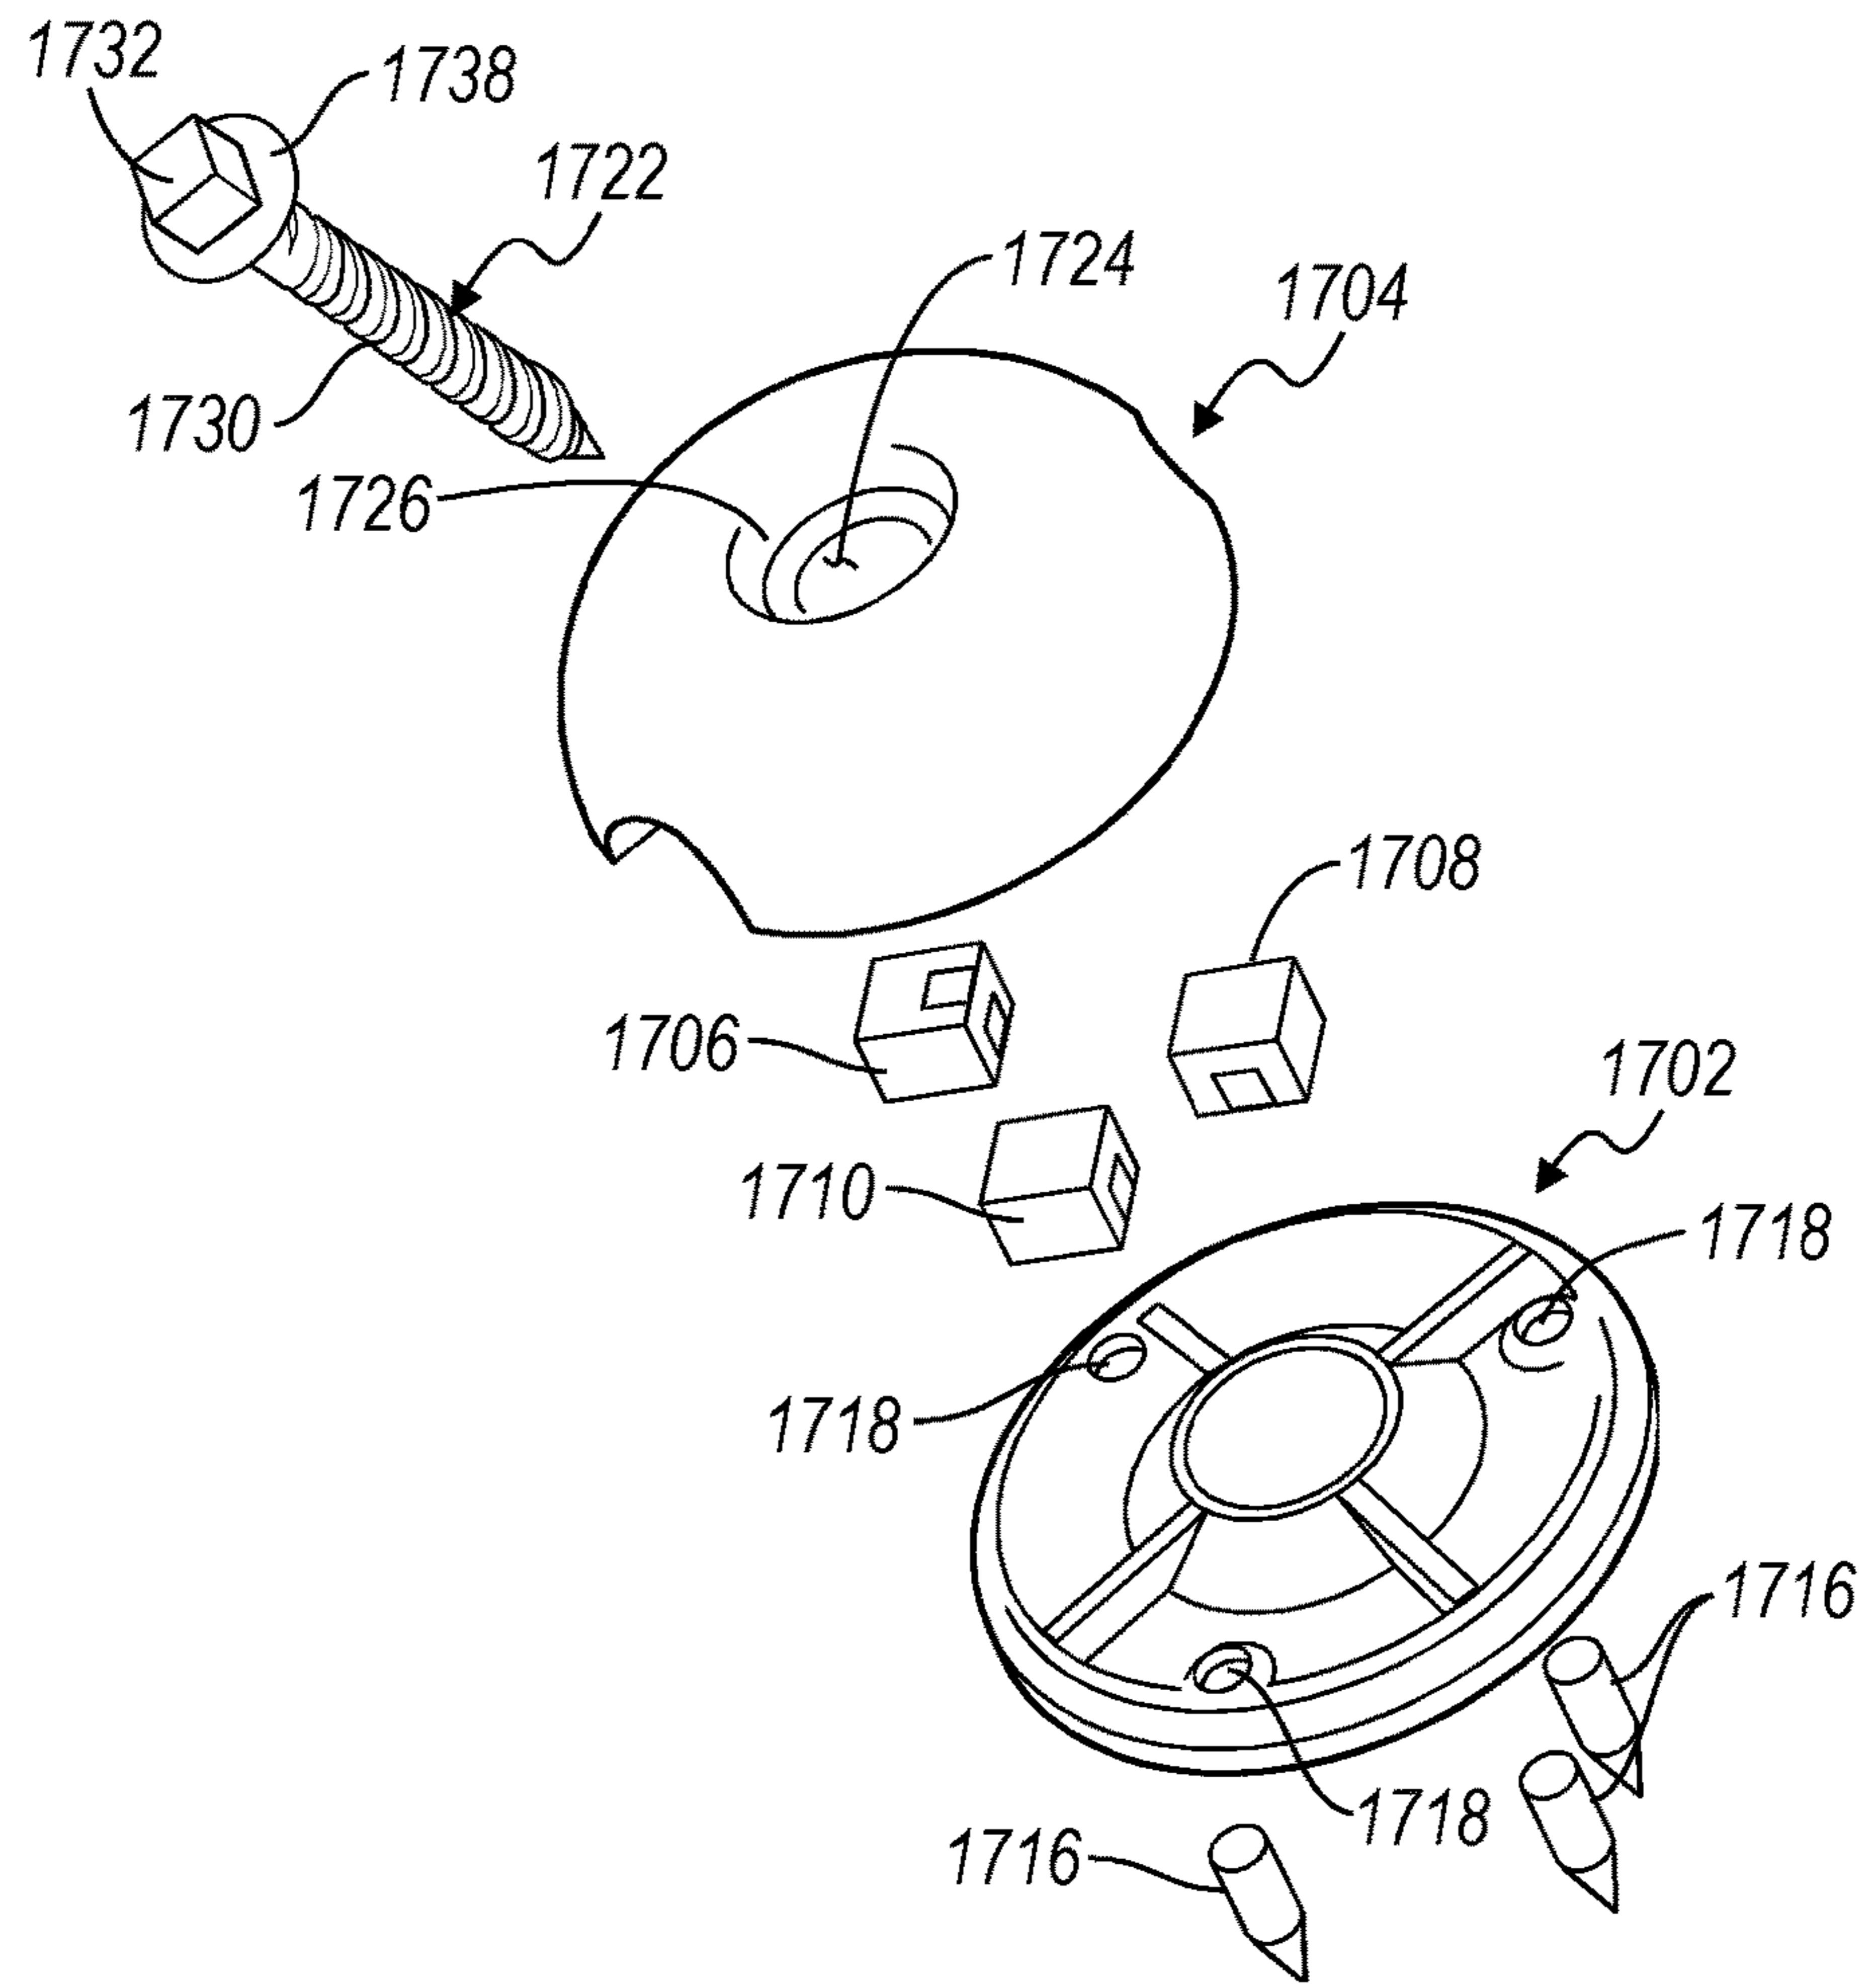


FIG. 77

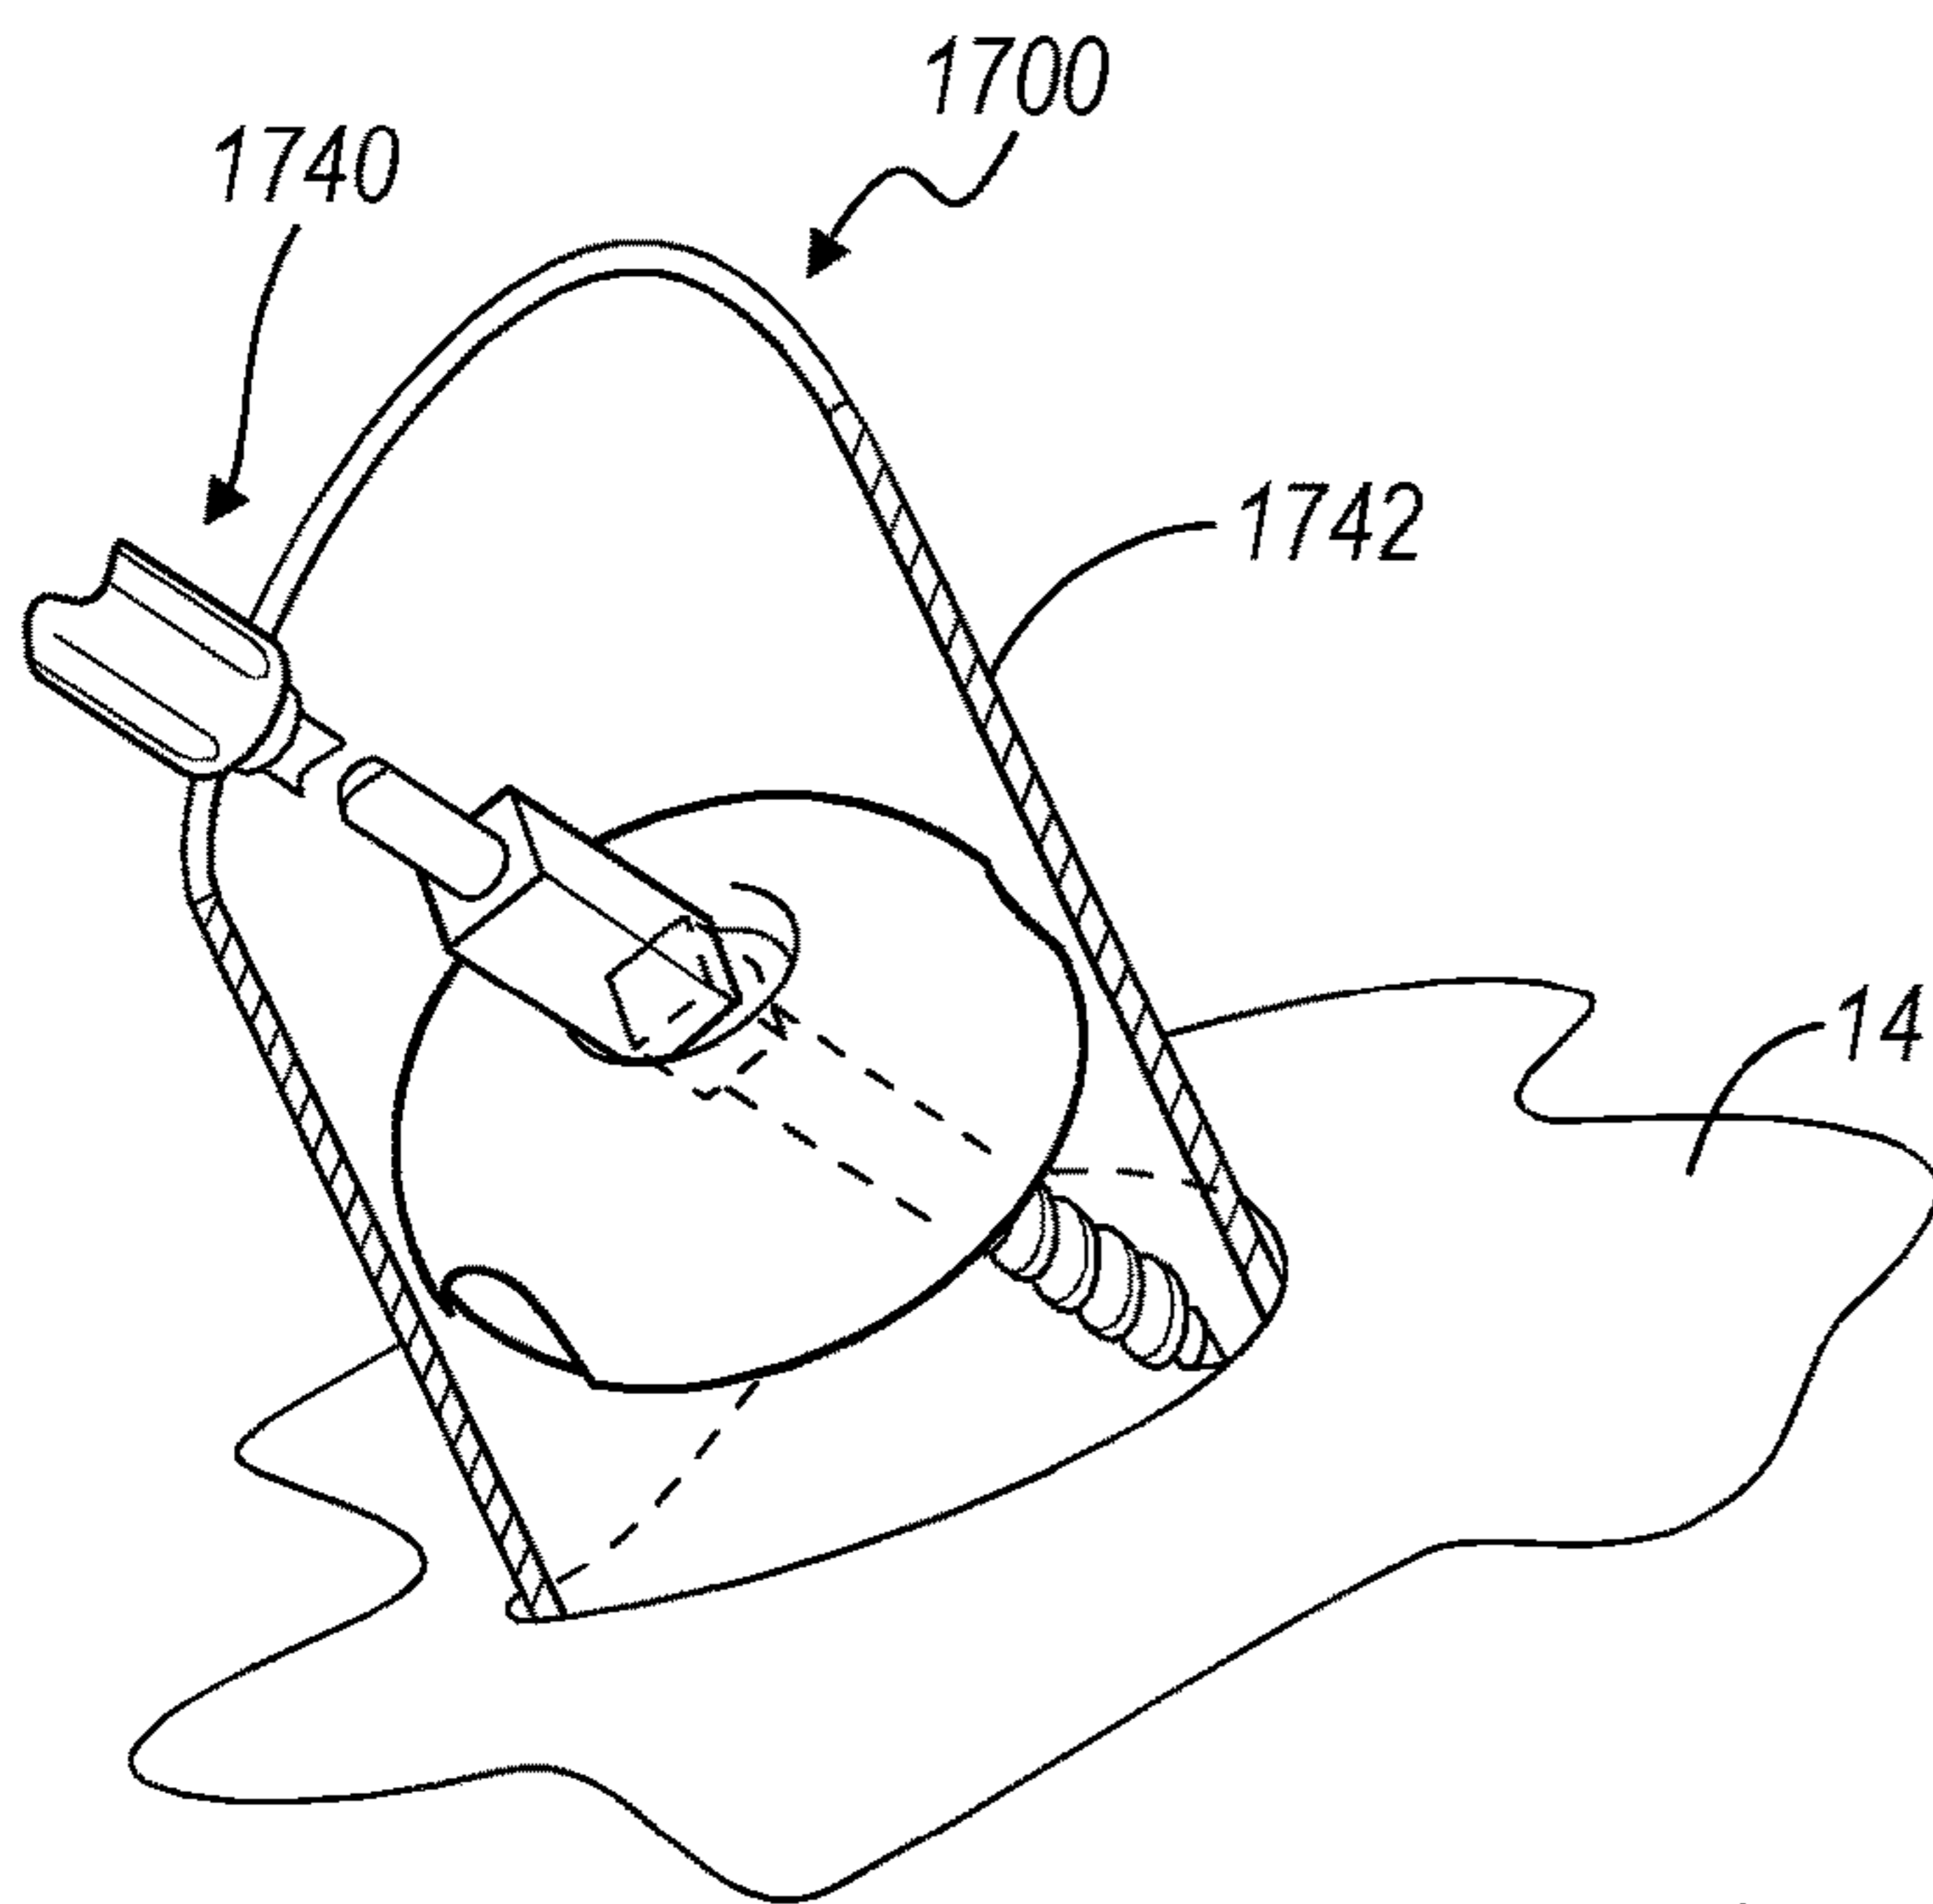


FIG. 78

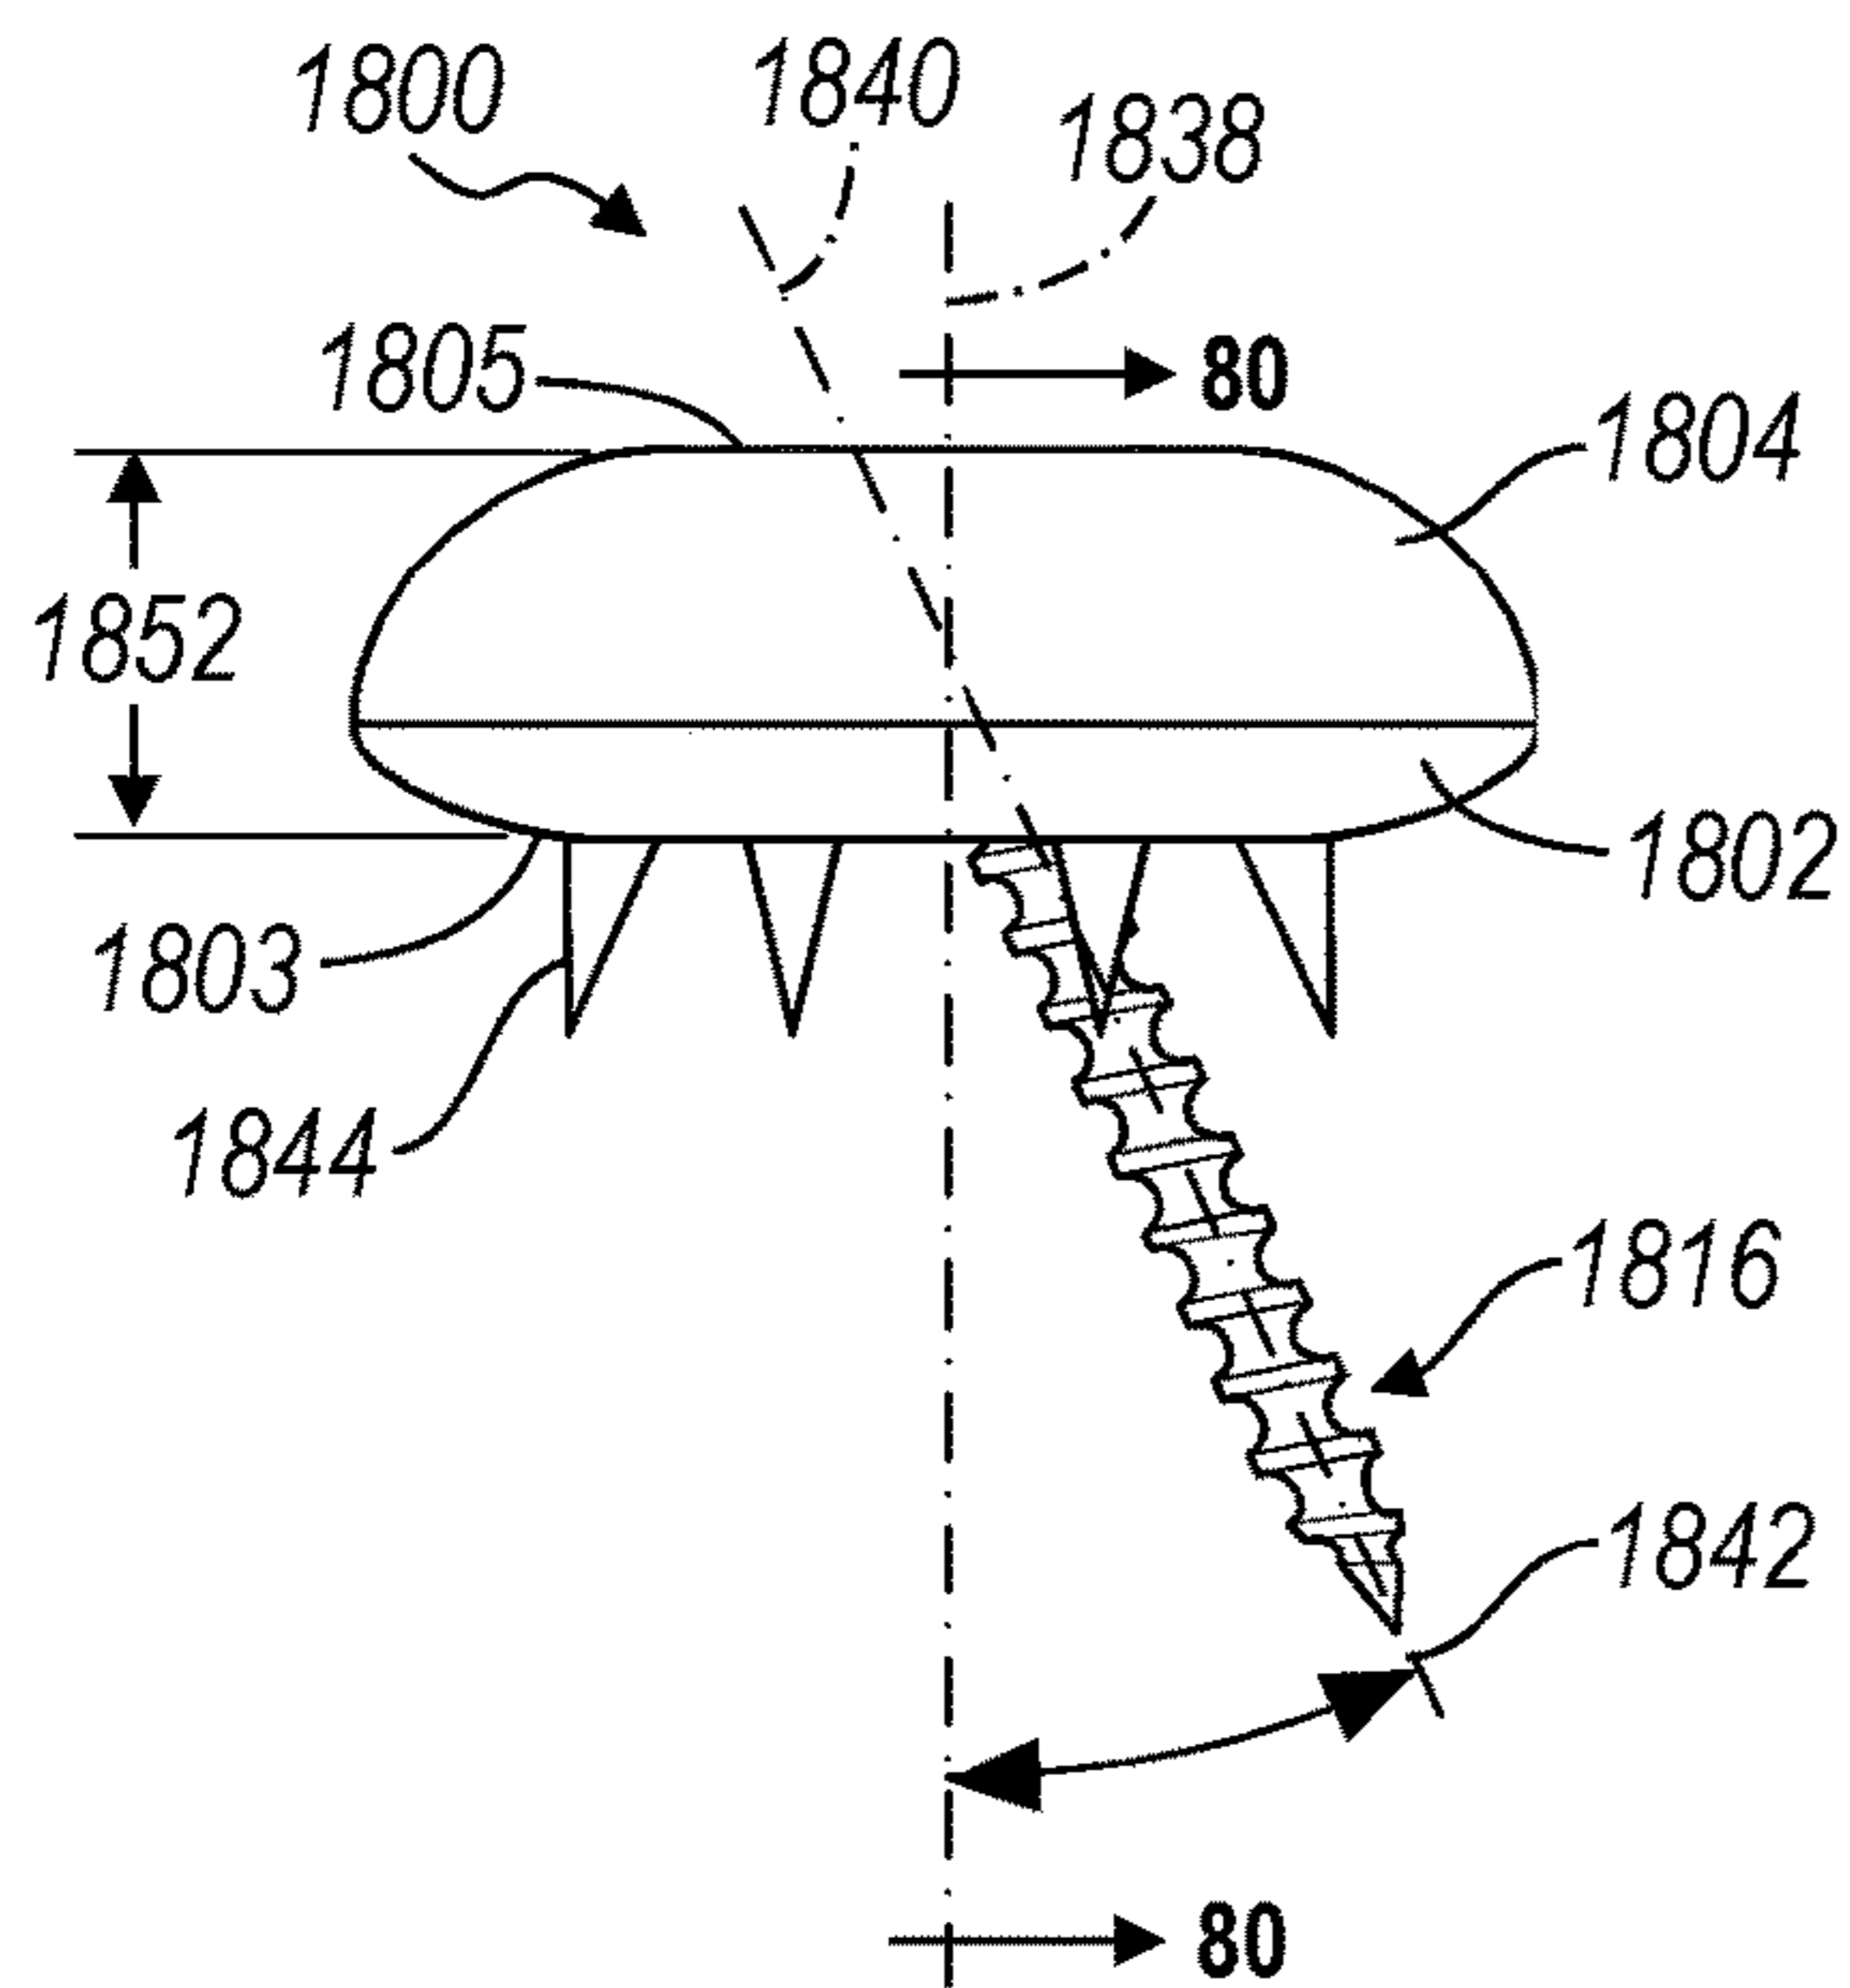


FIG. 79

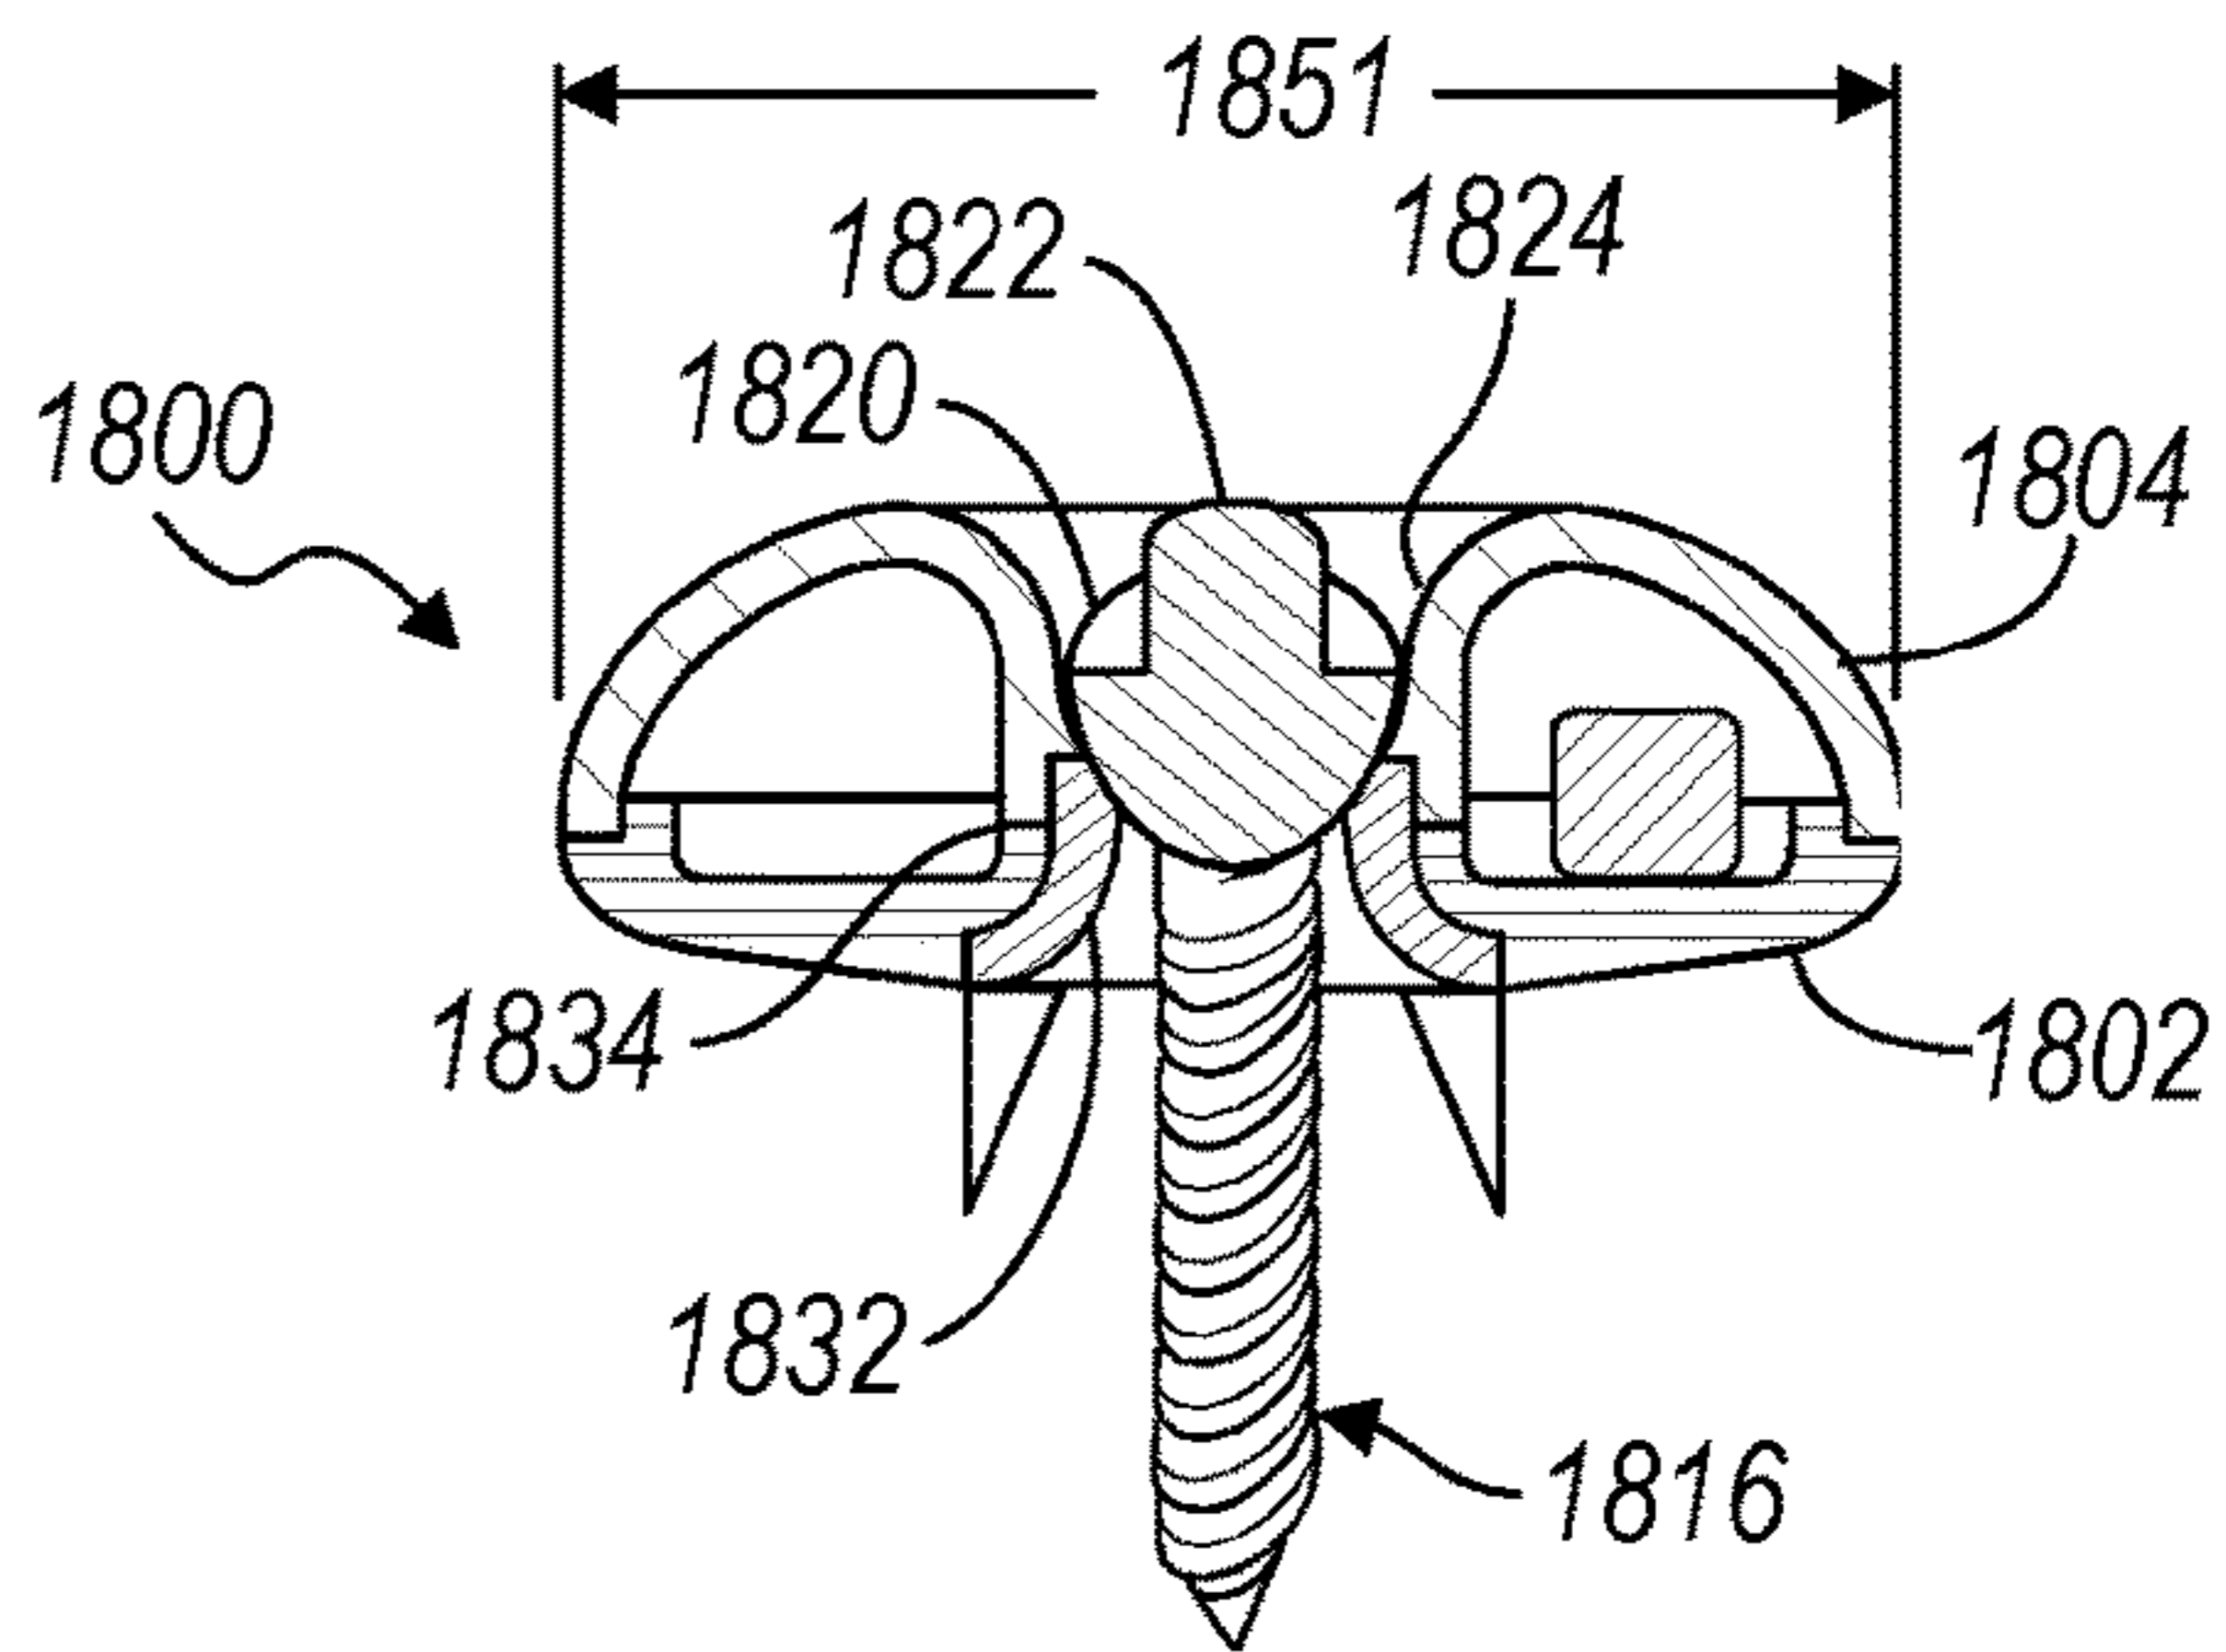


FIG. 80

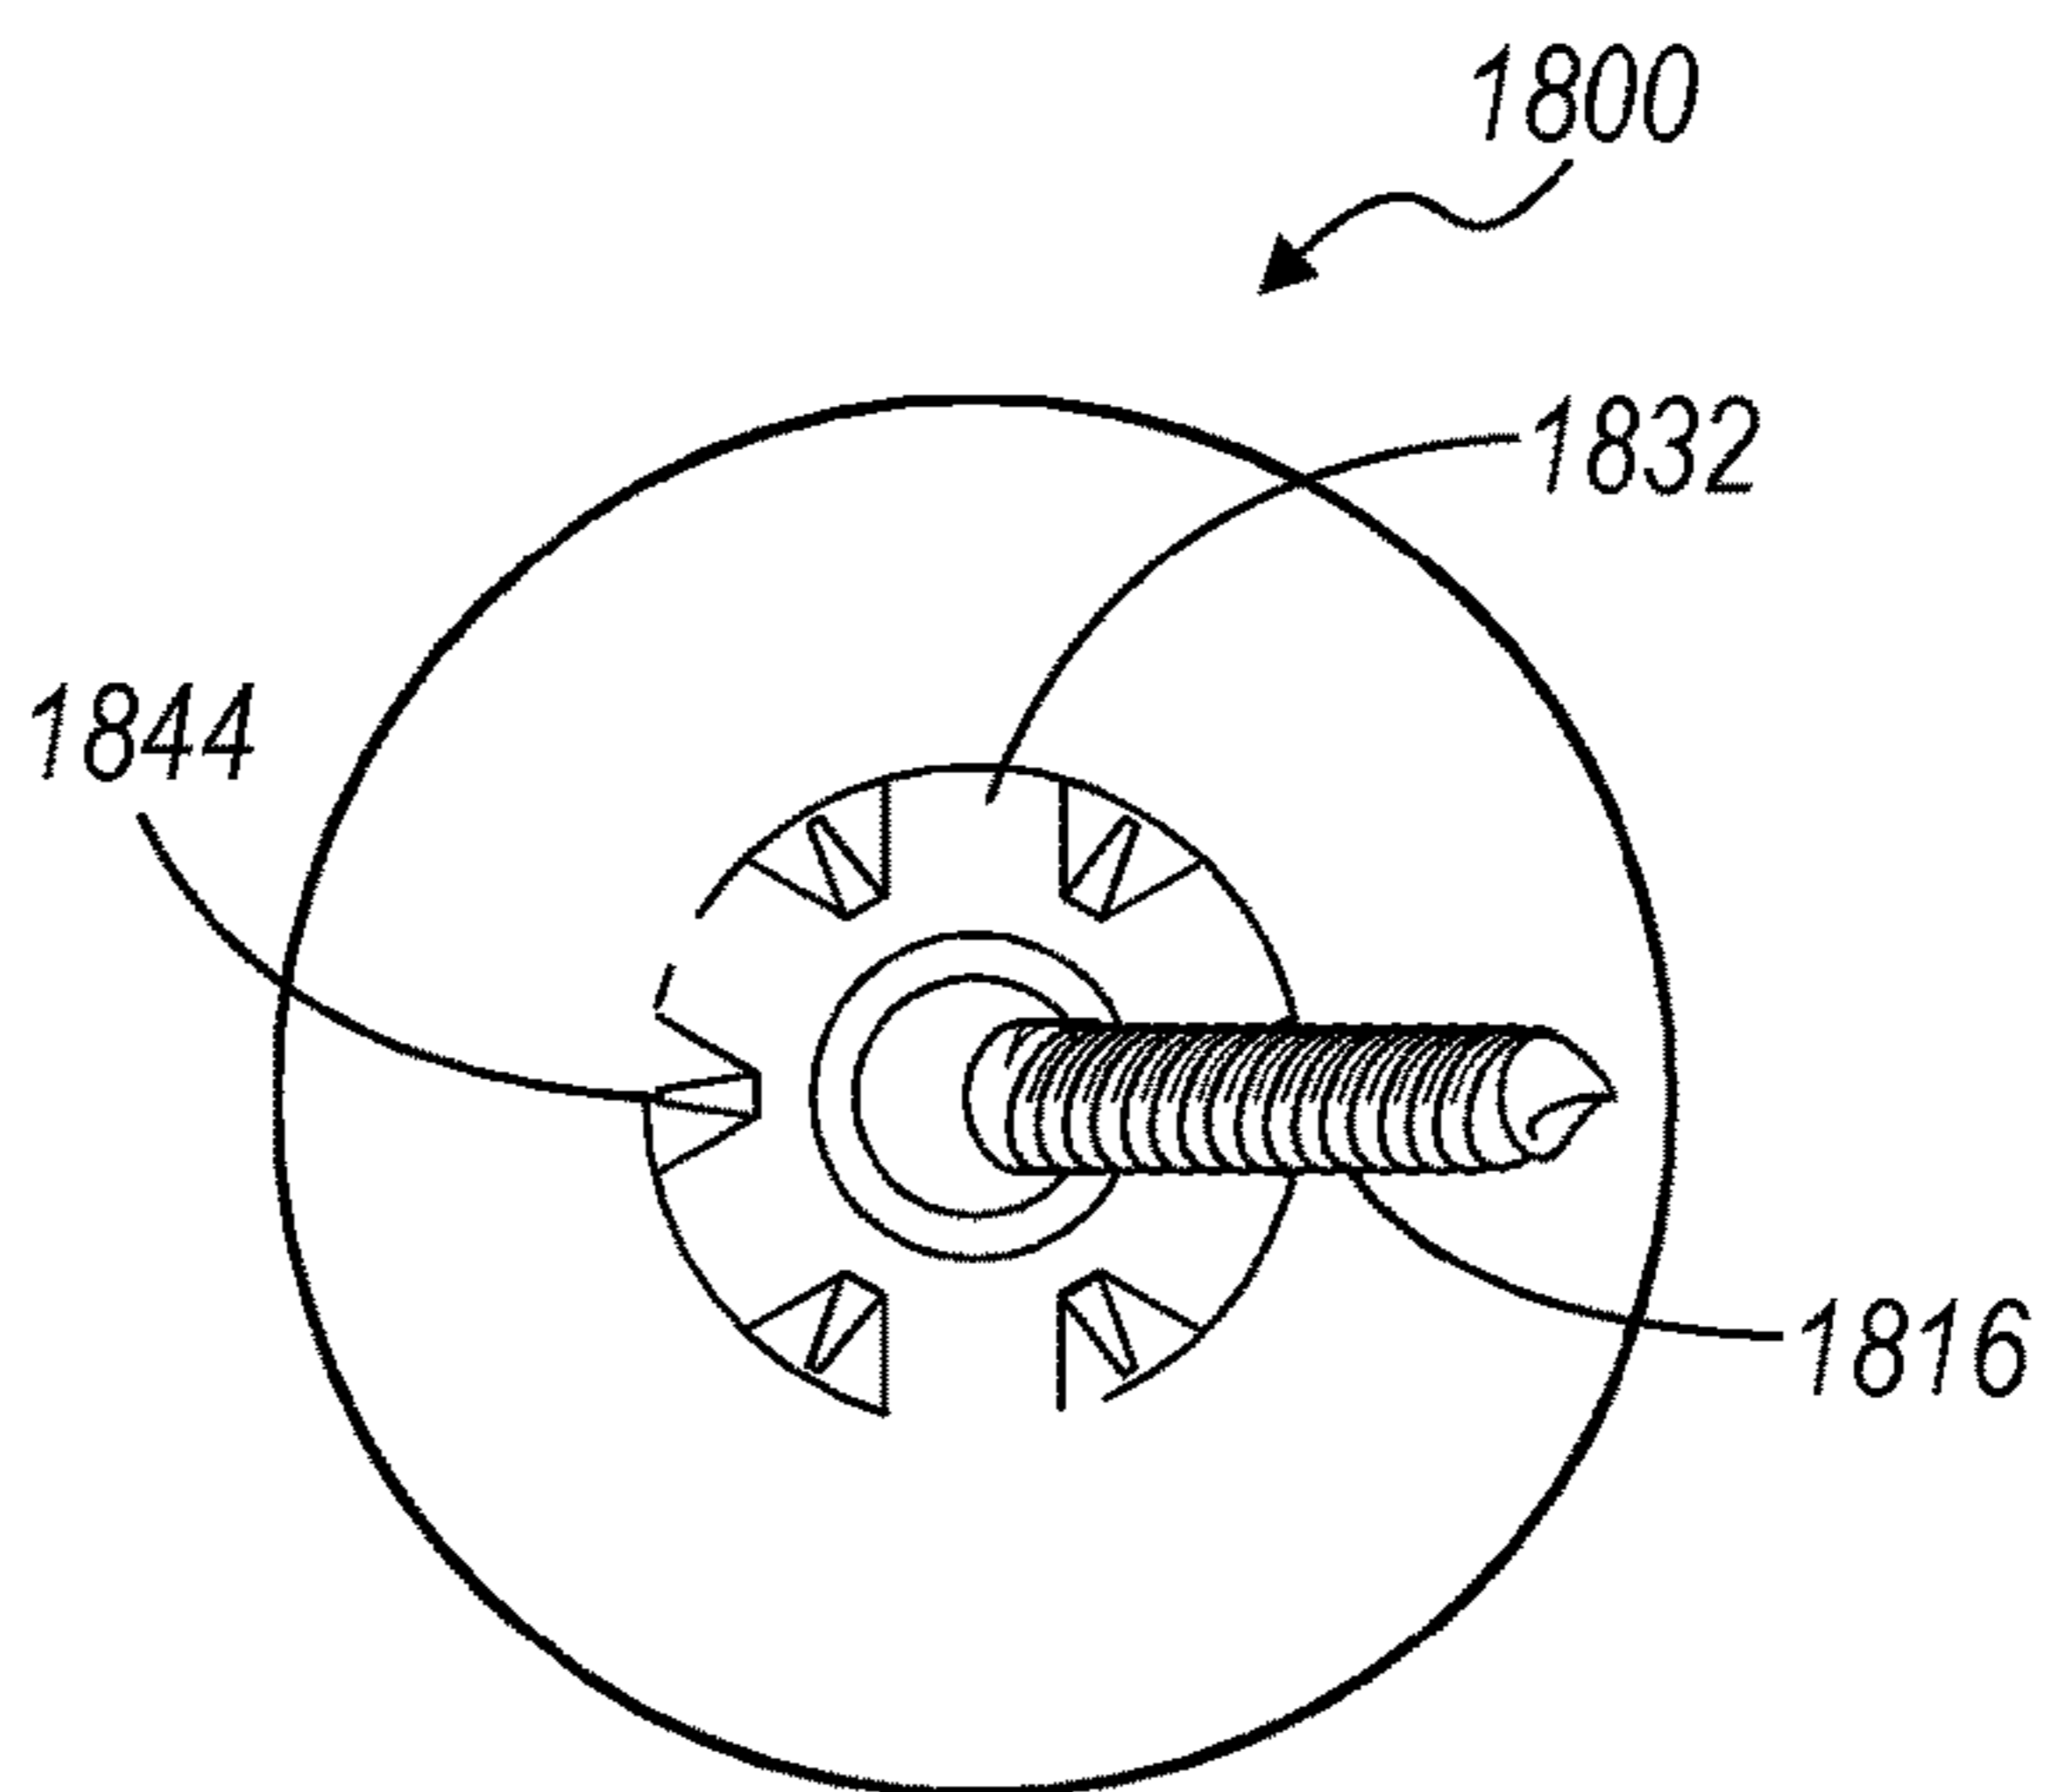


FIG. 81

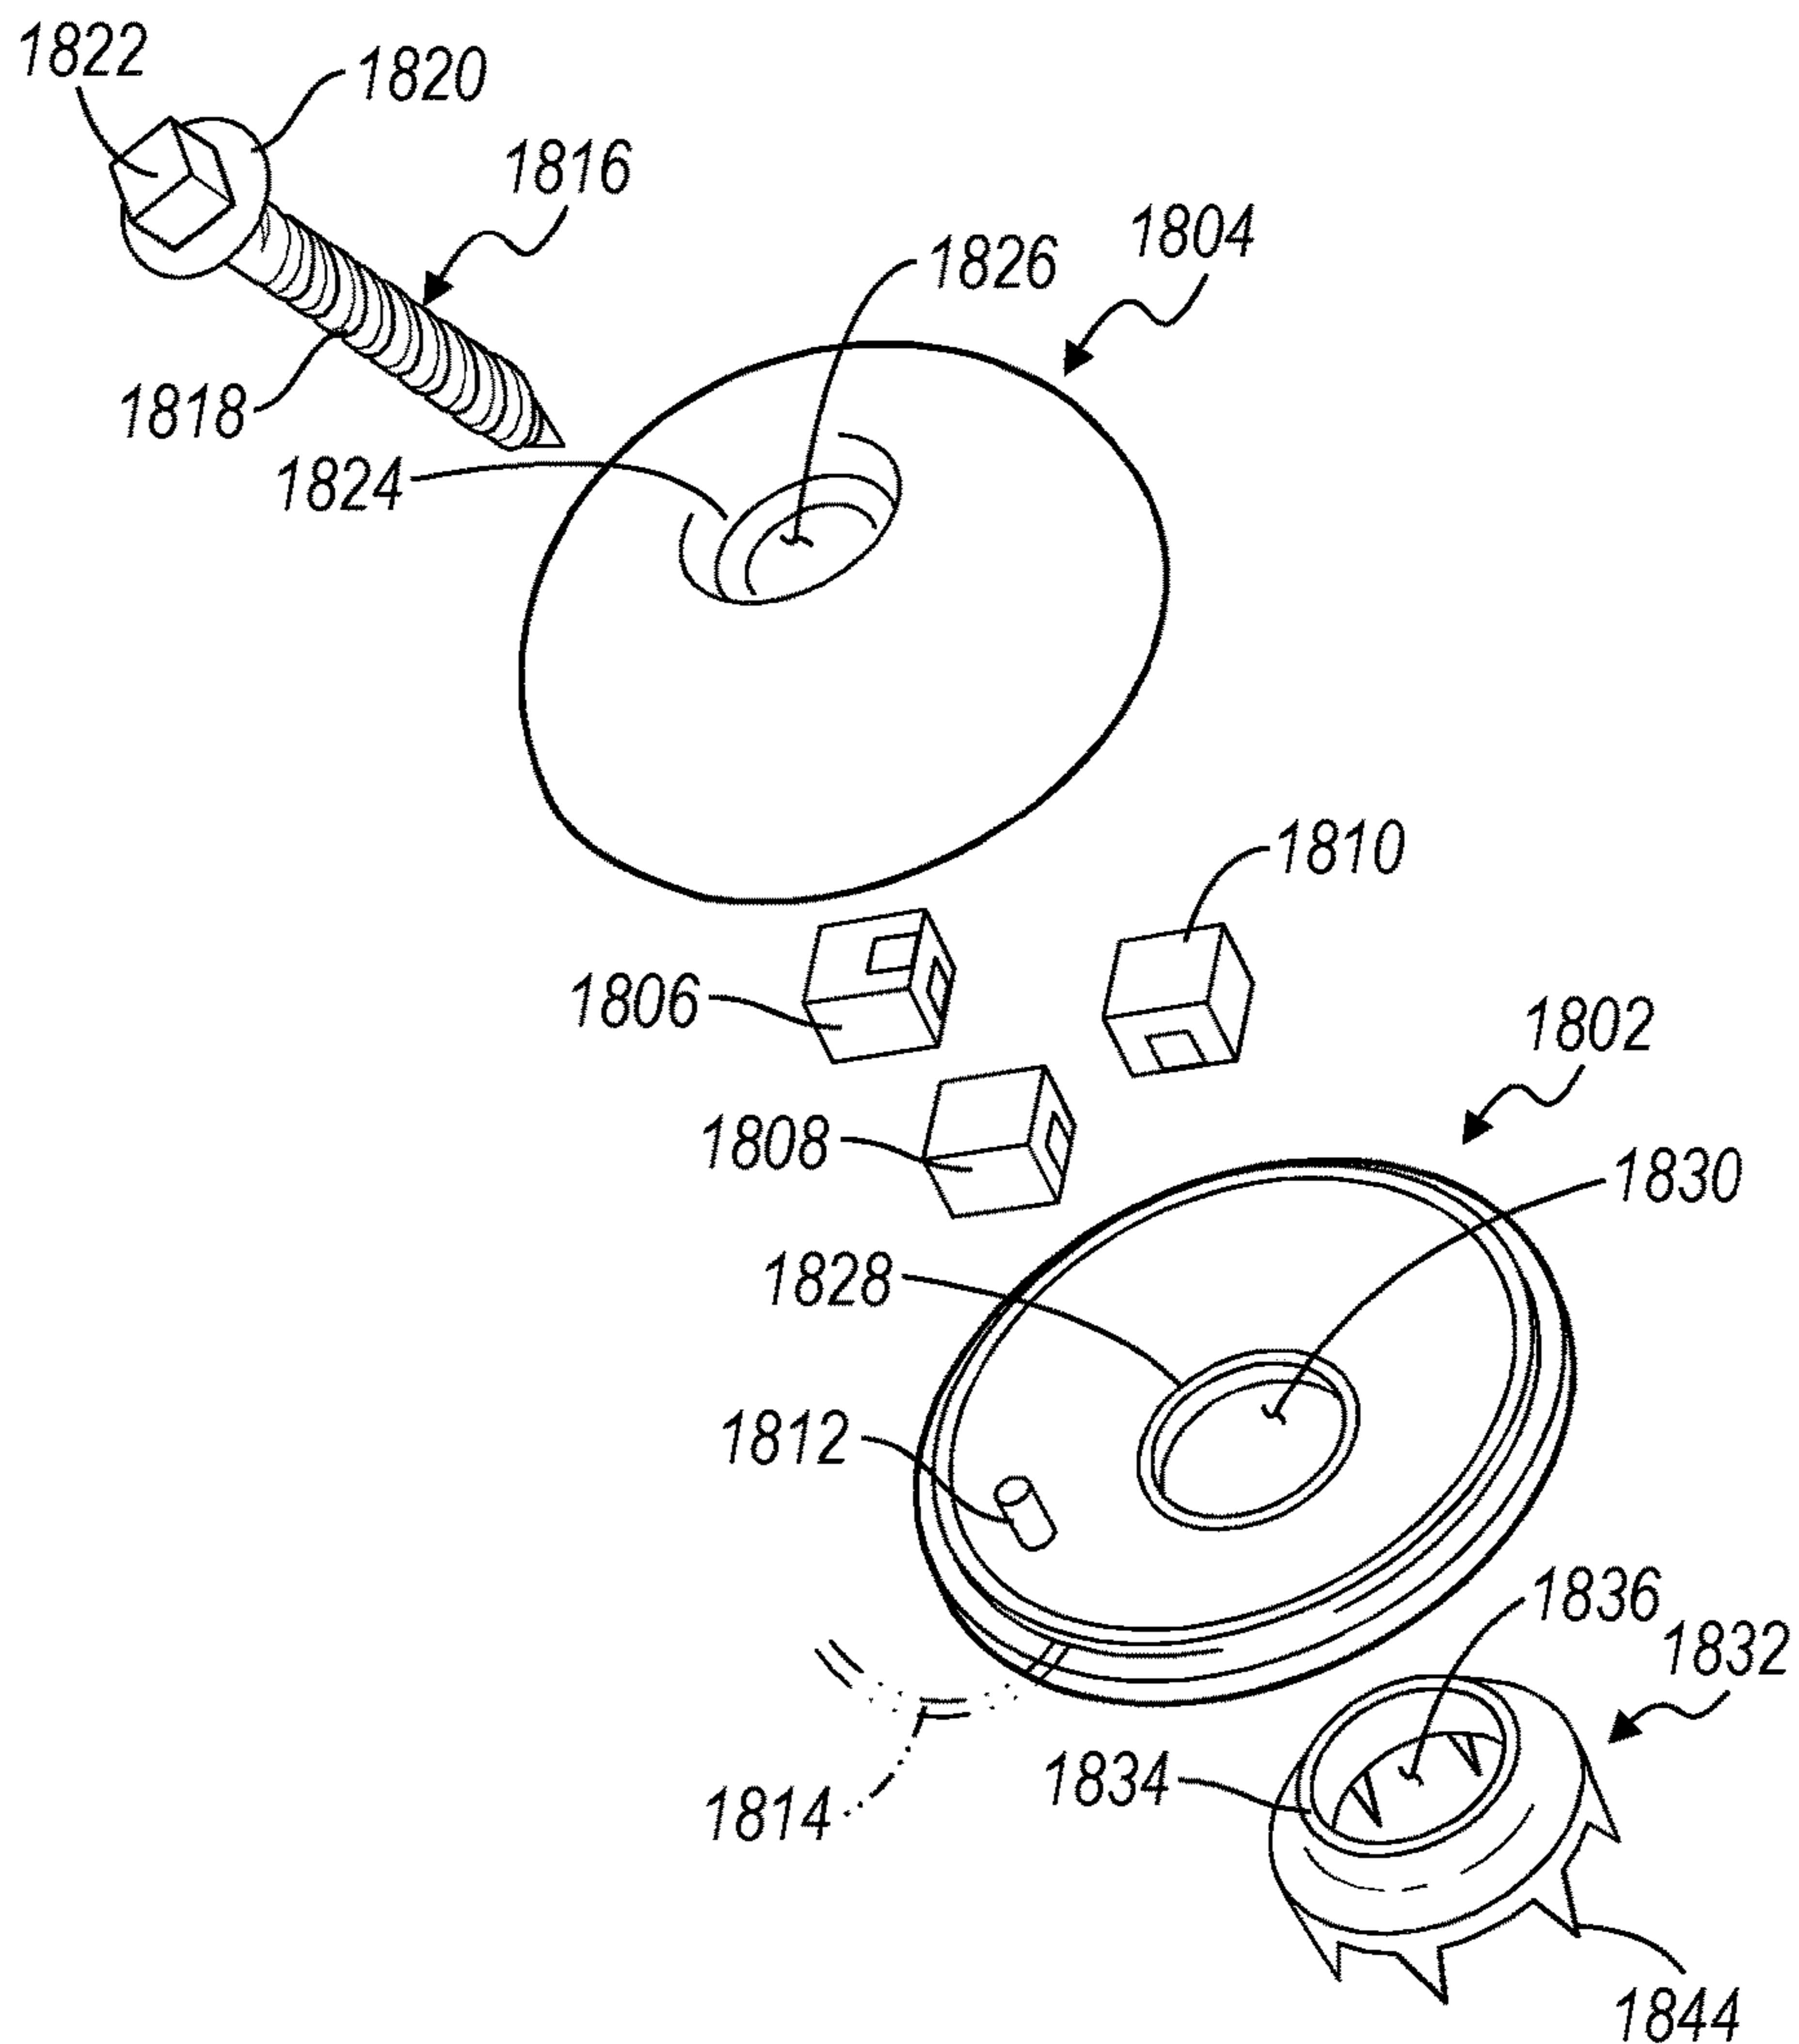


FIG. 82

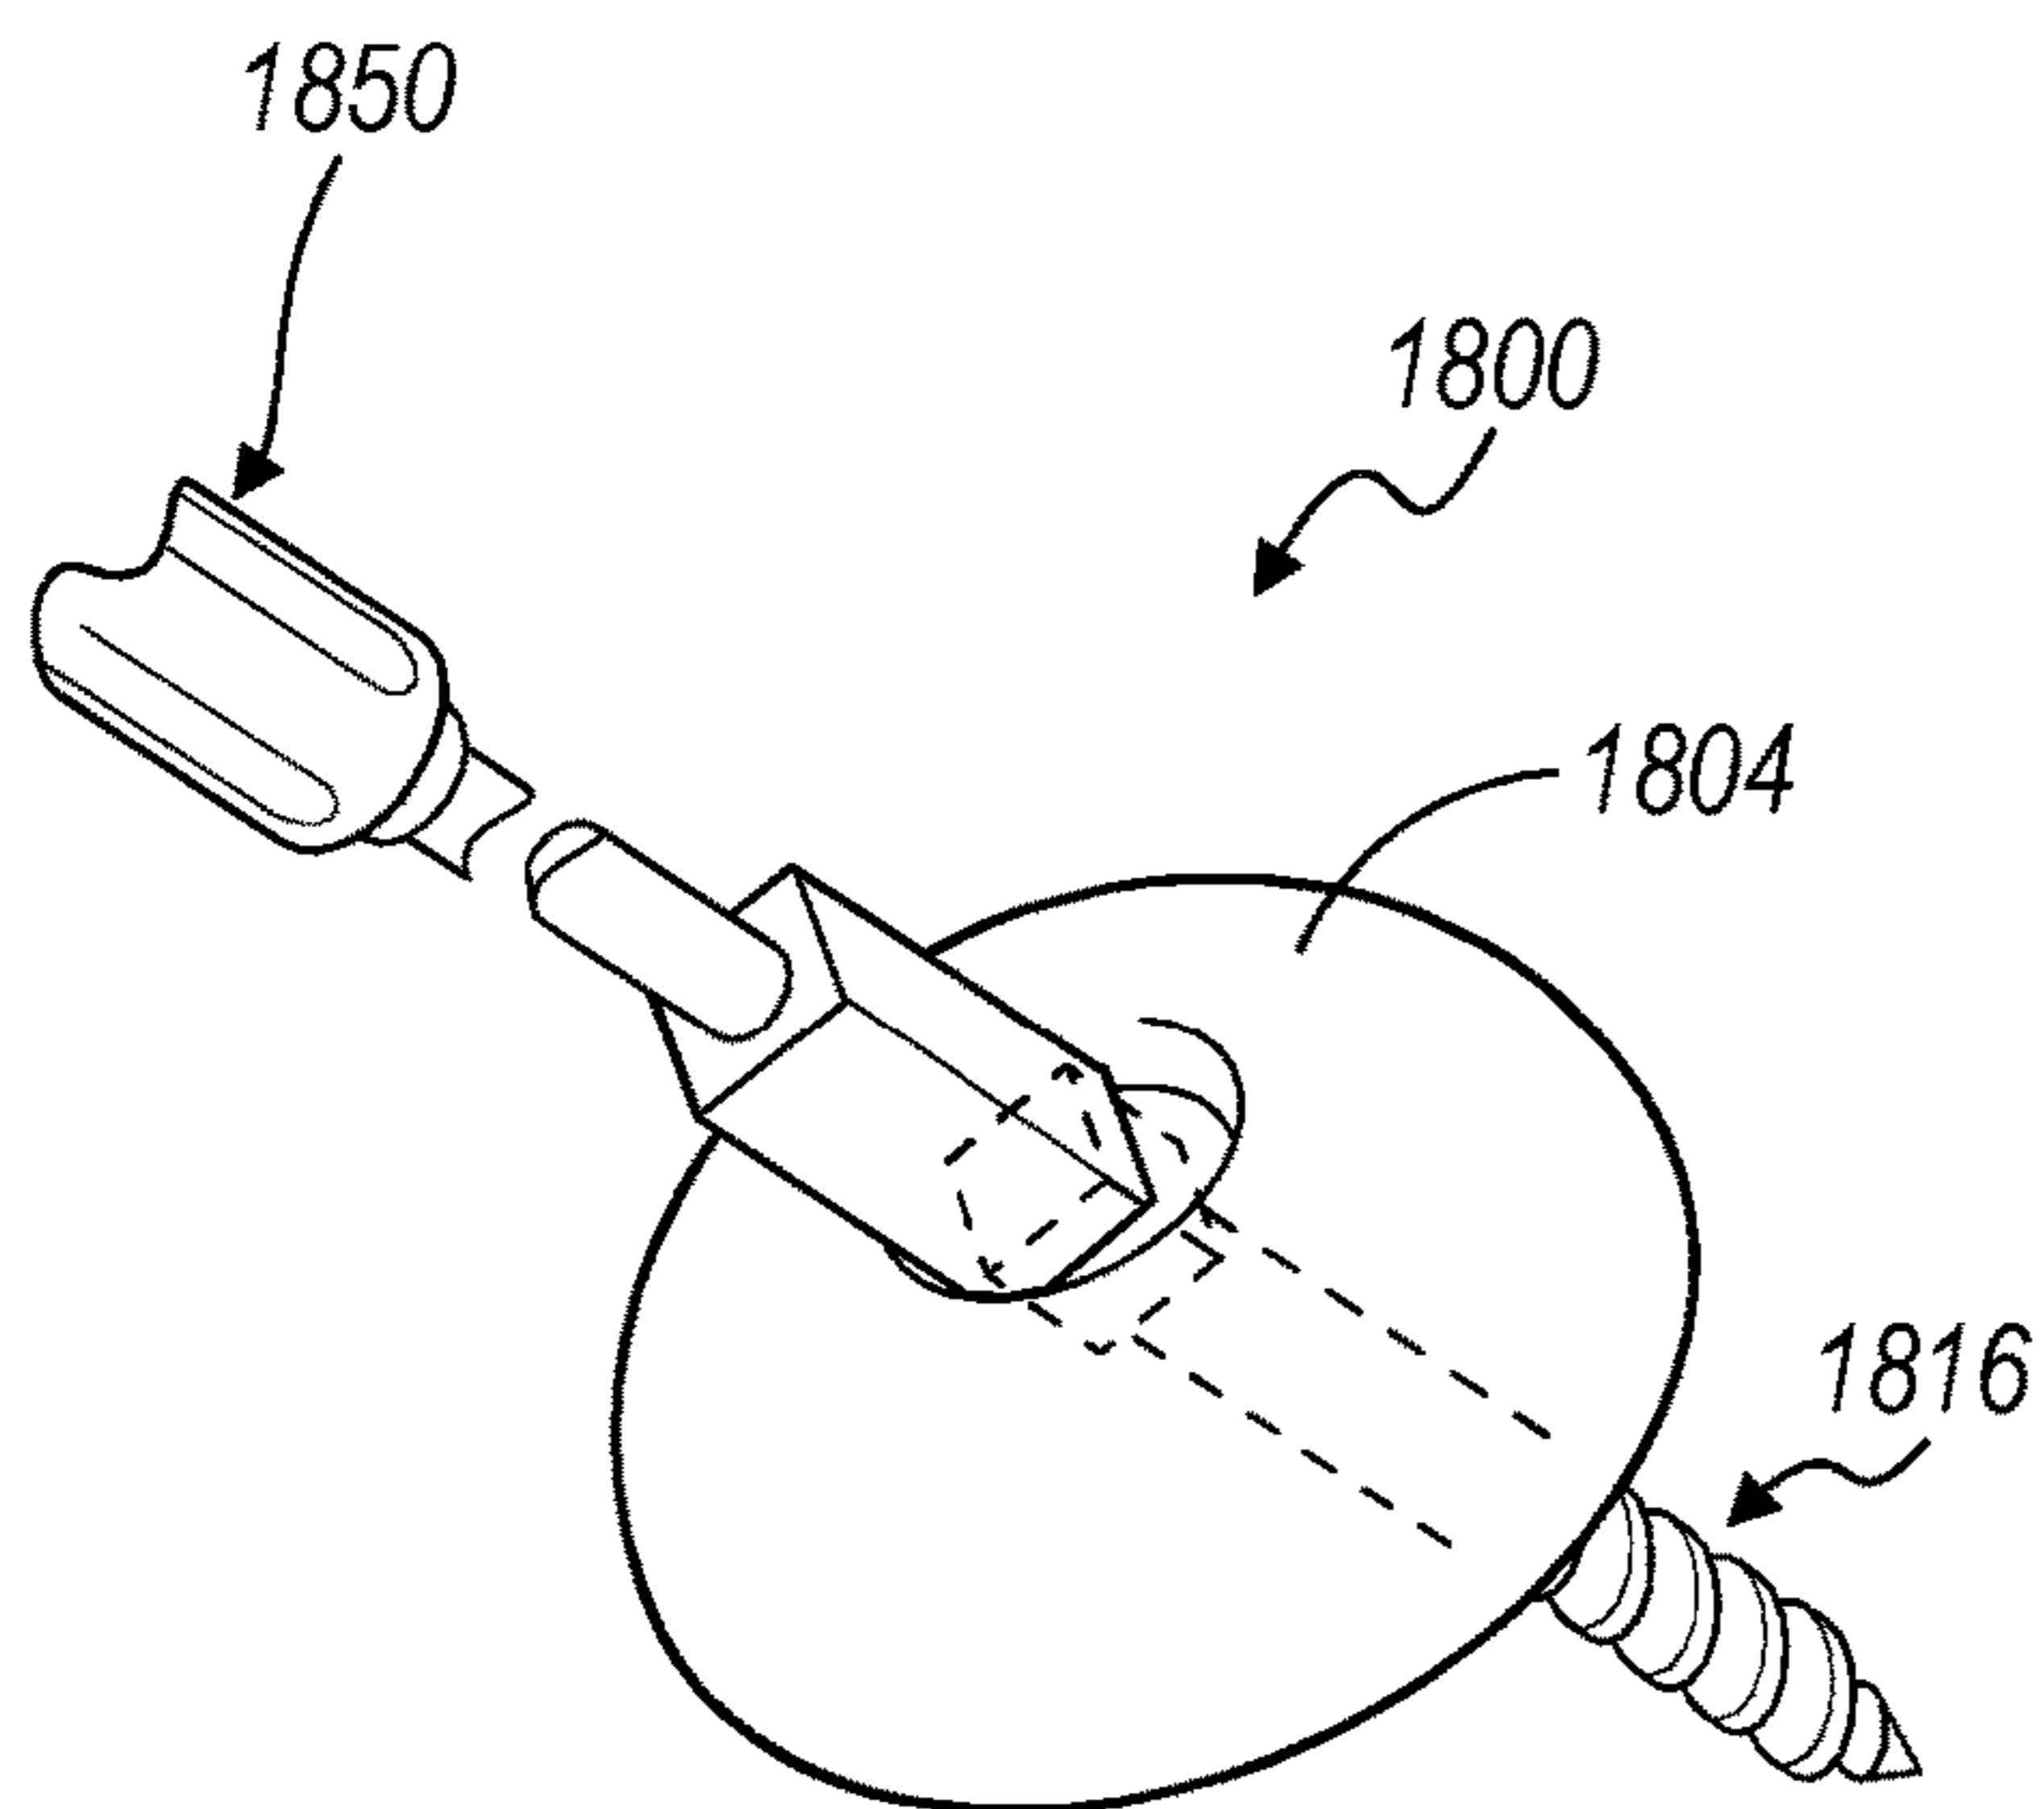


FIG. 83

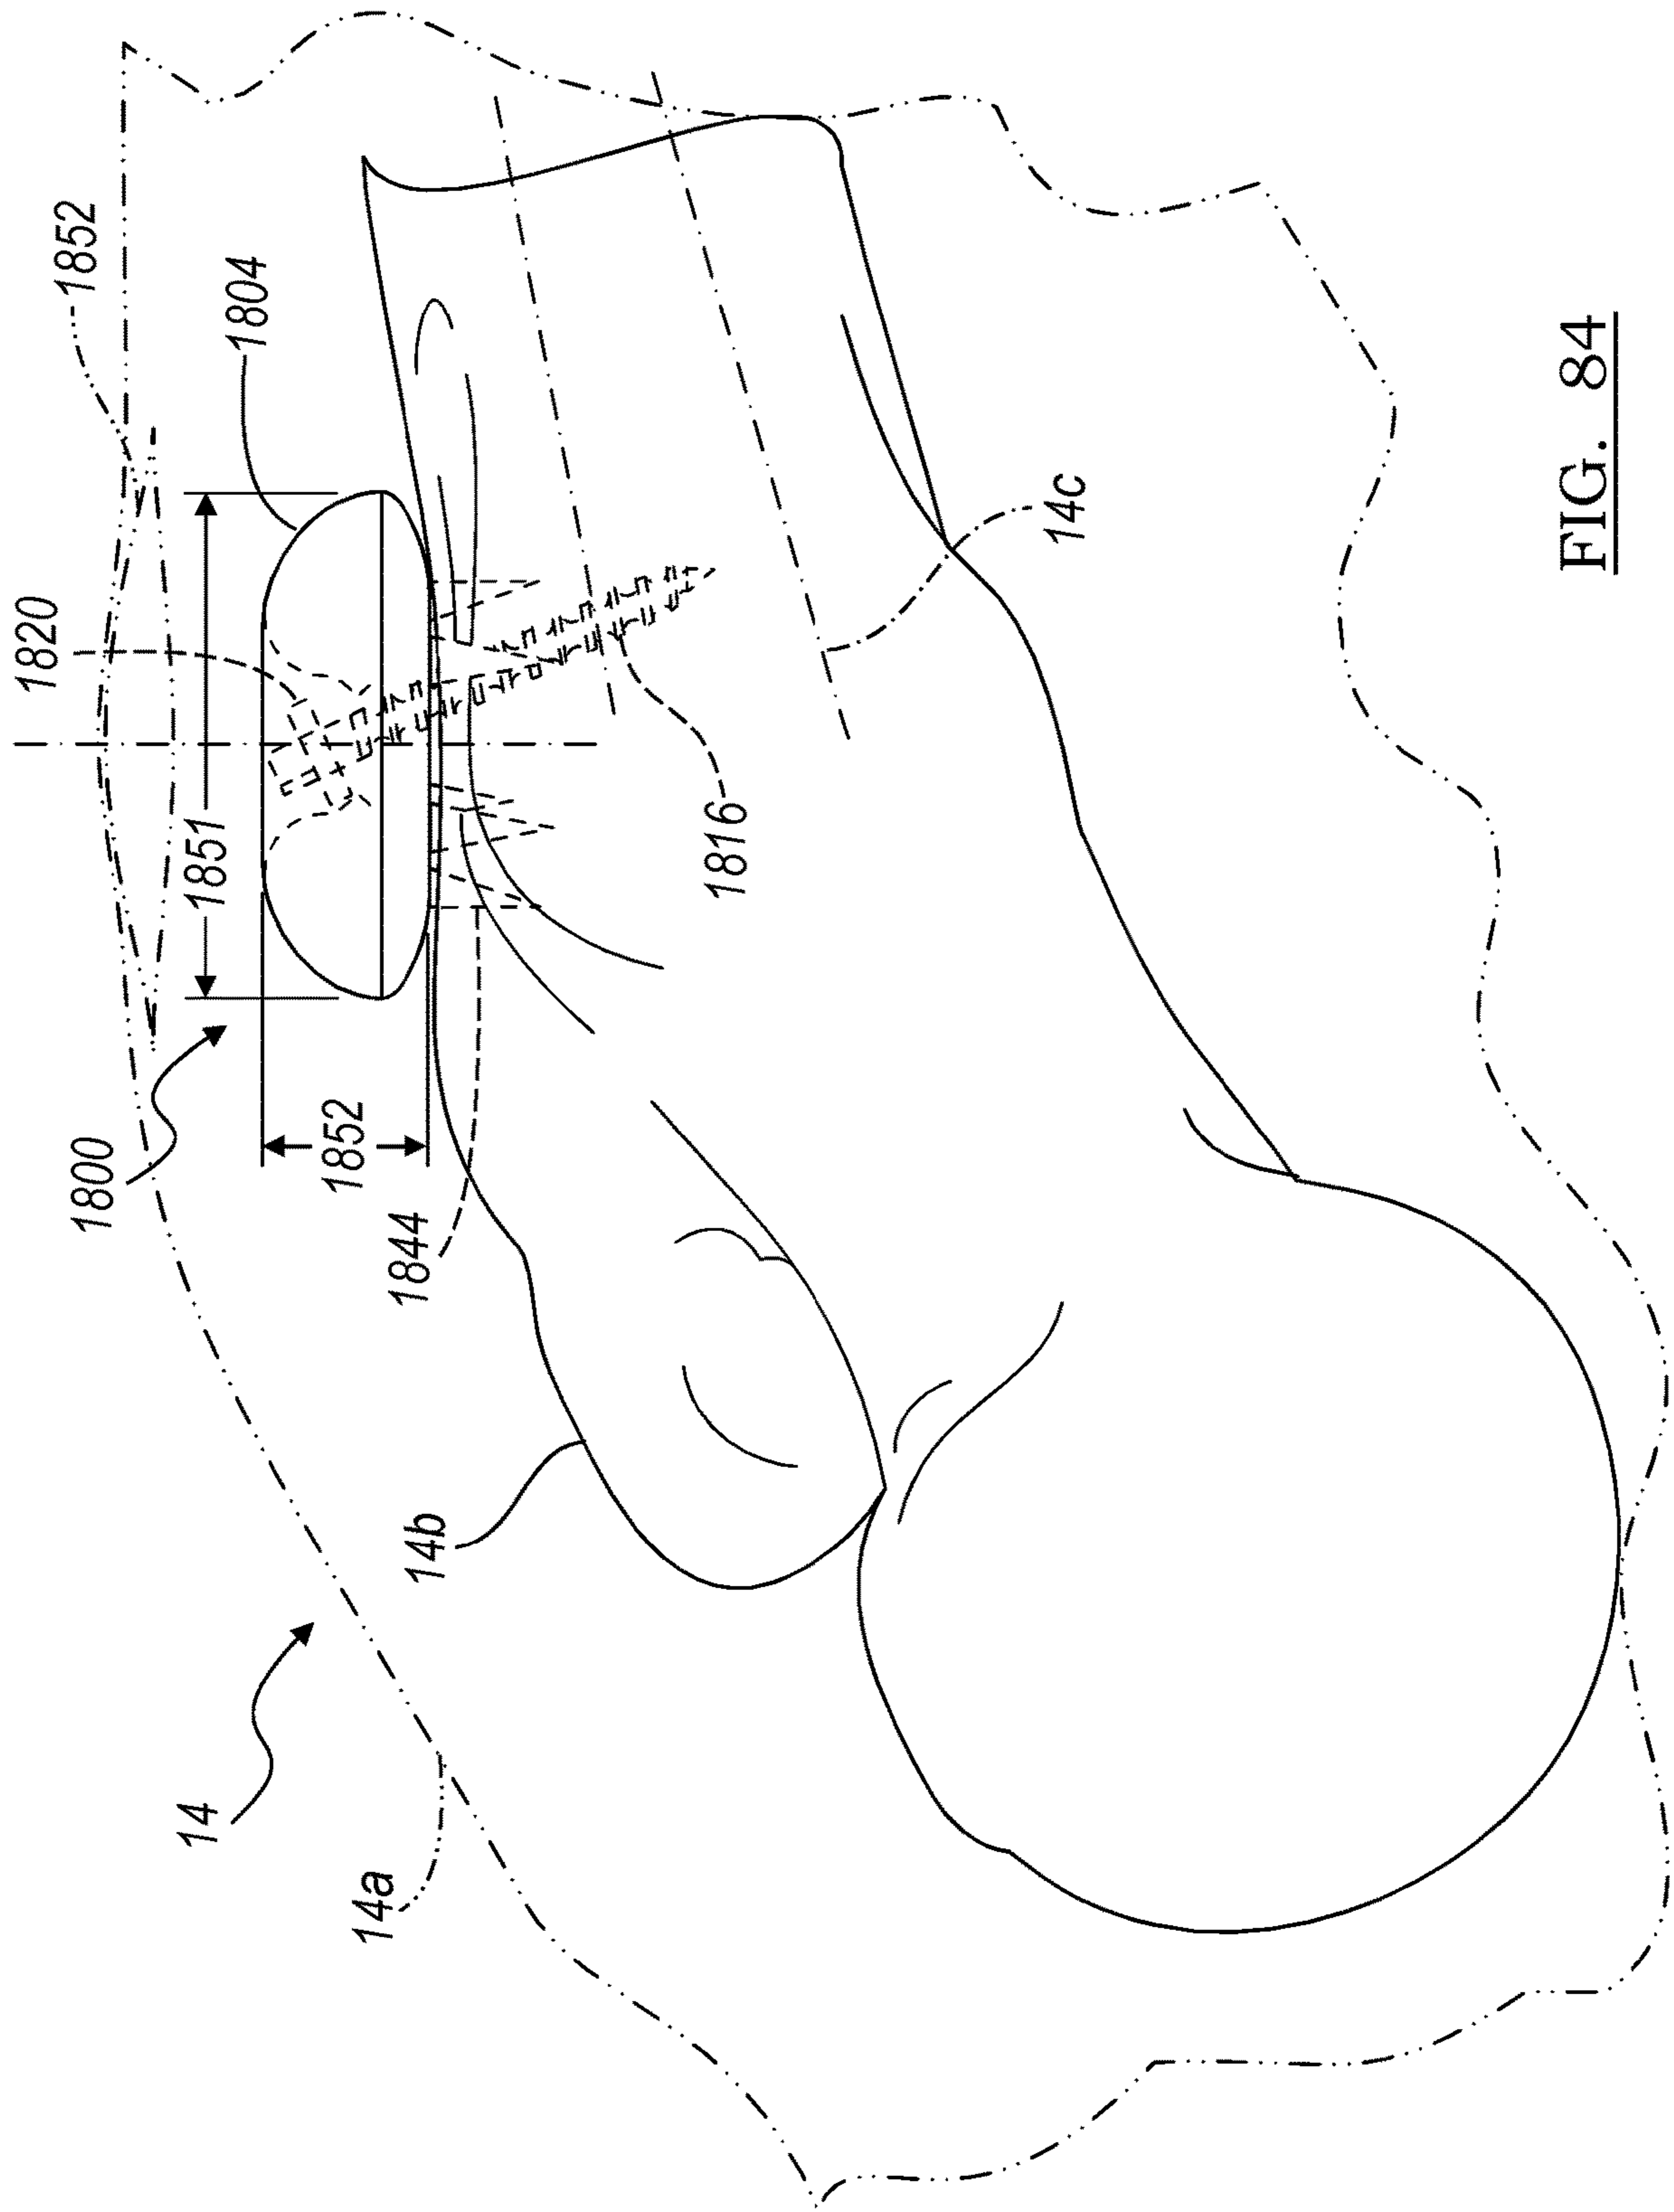


FIG. 84

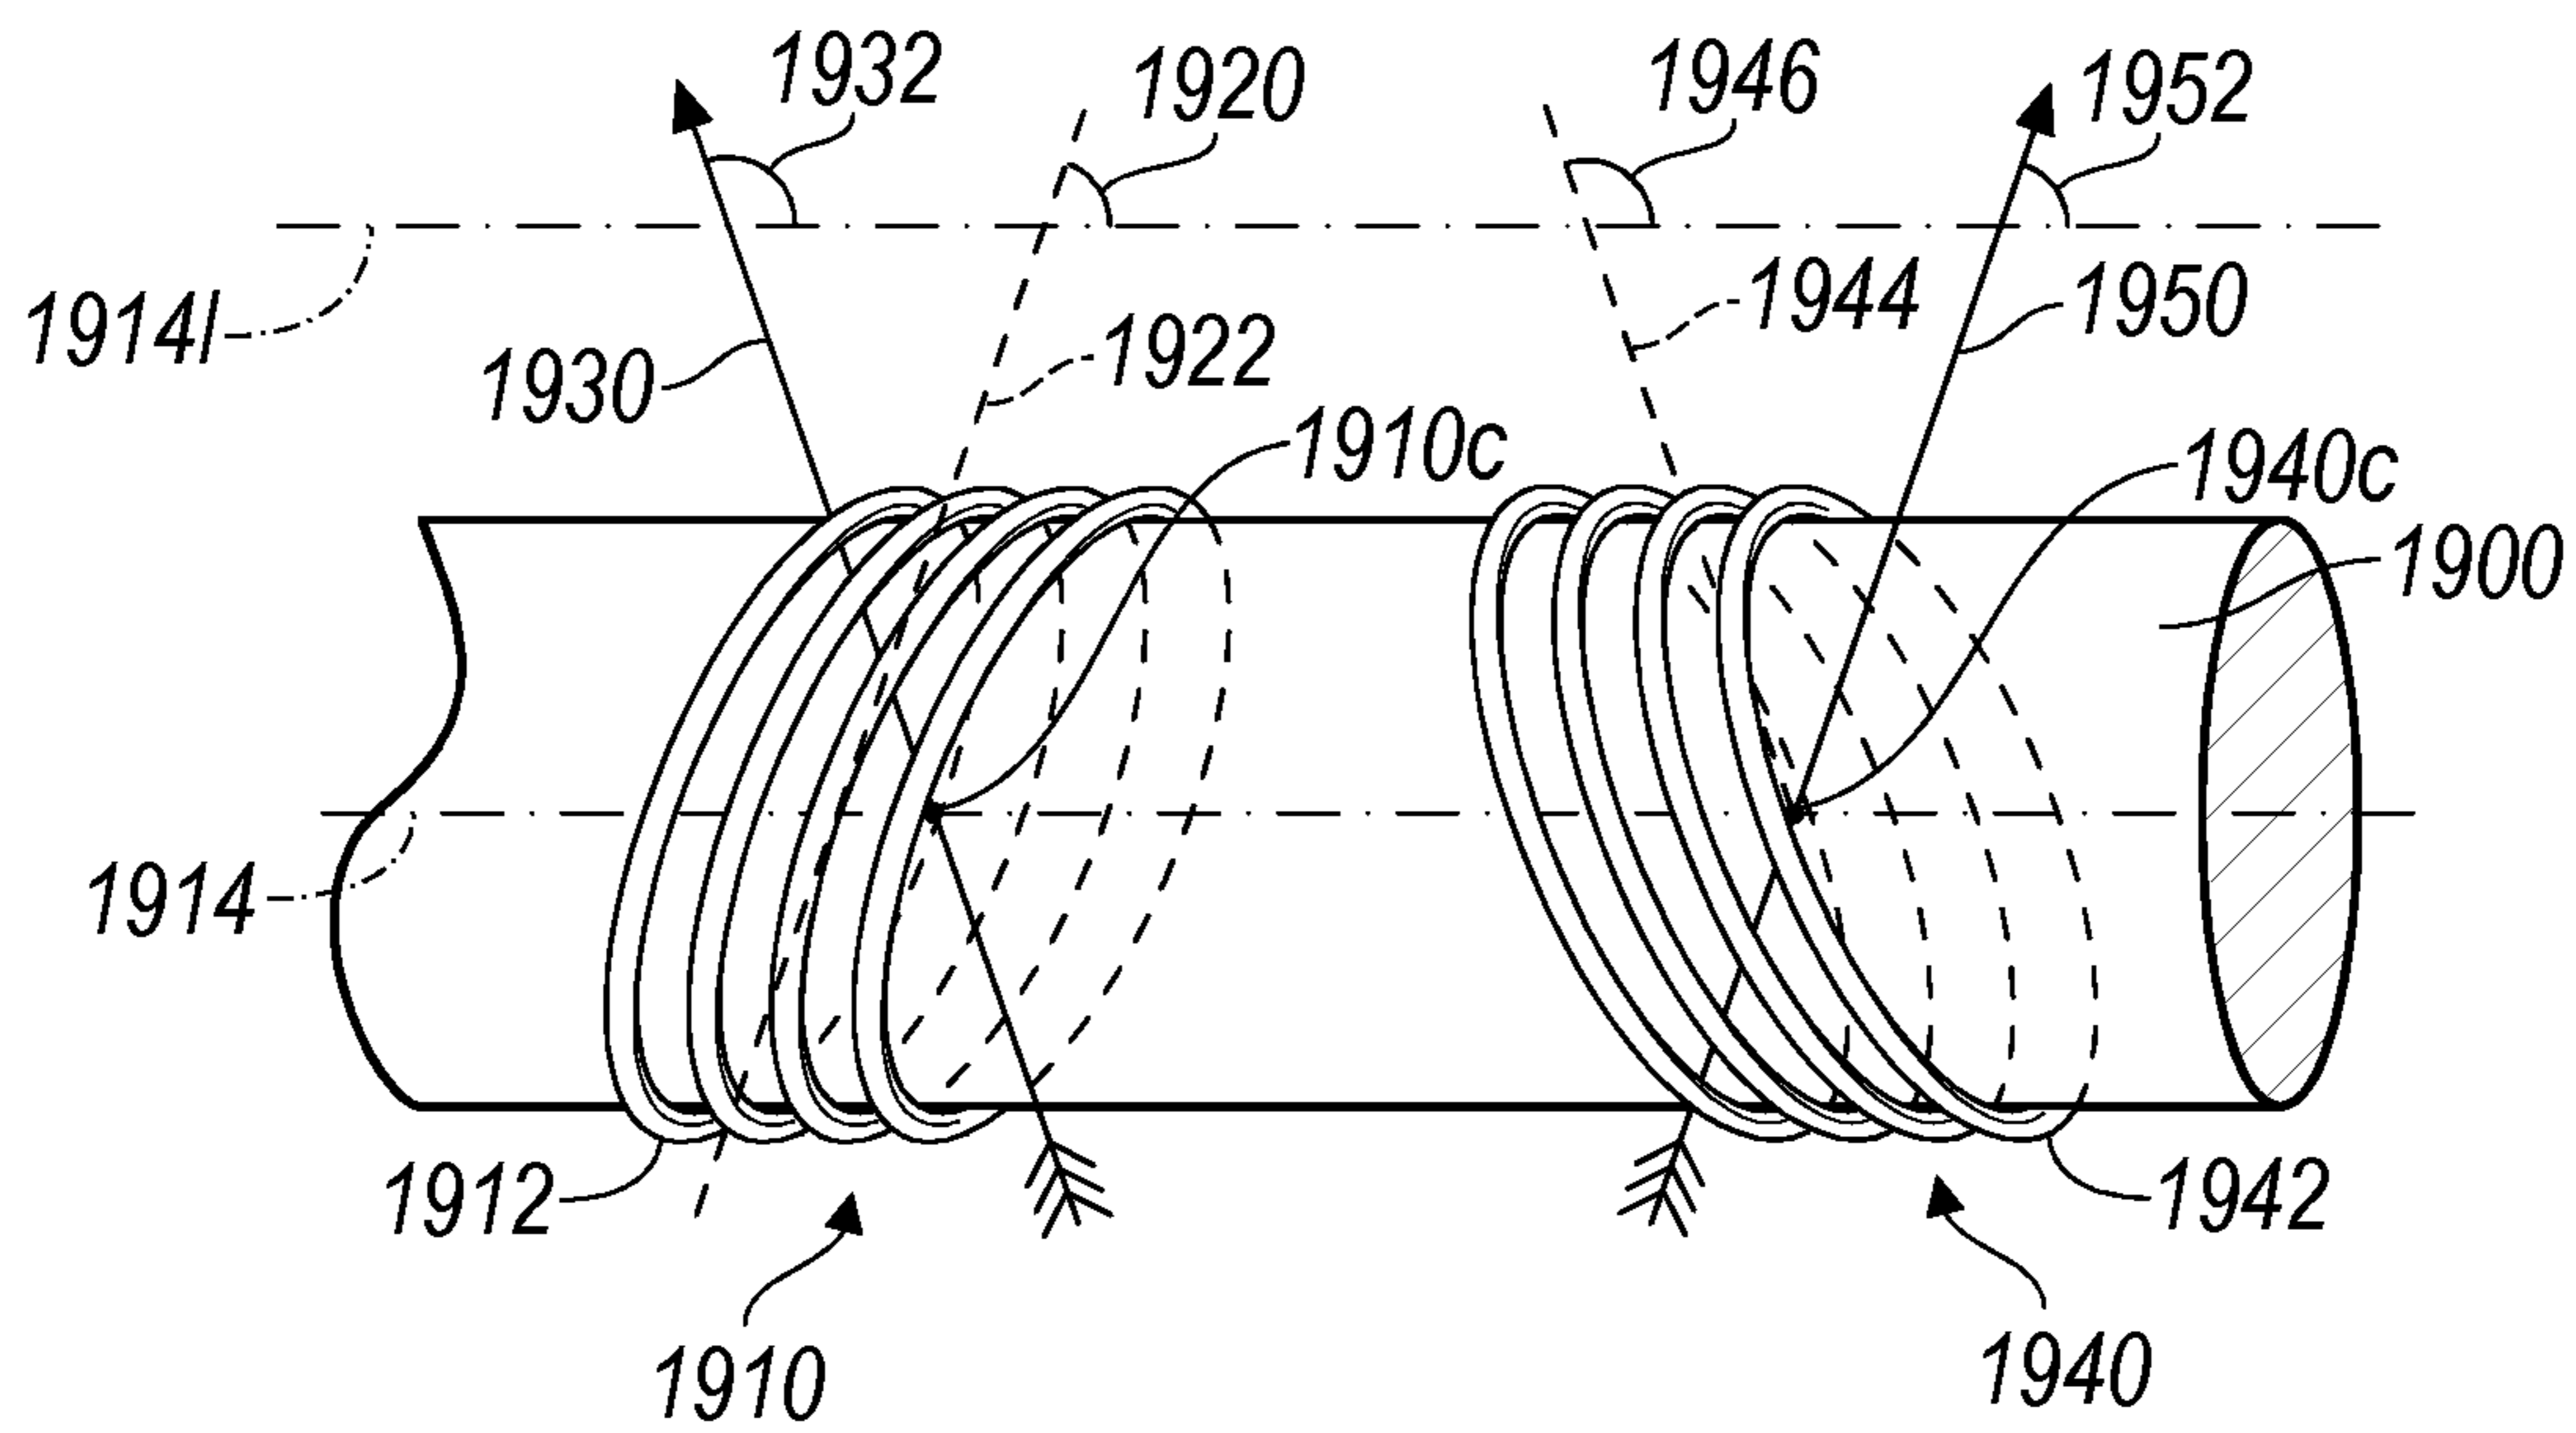


FIG. 85

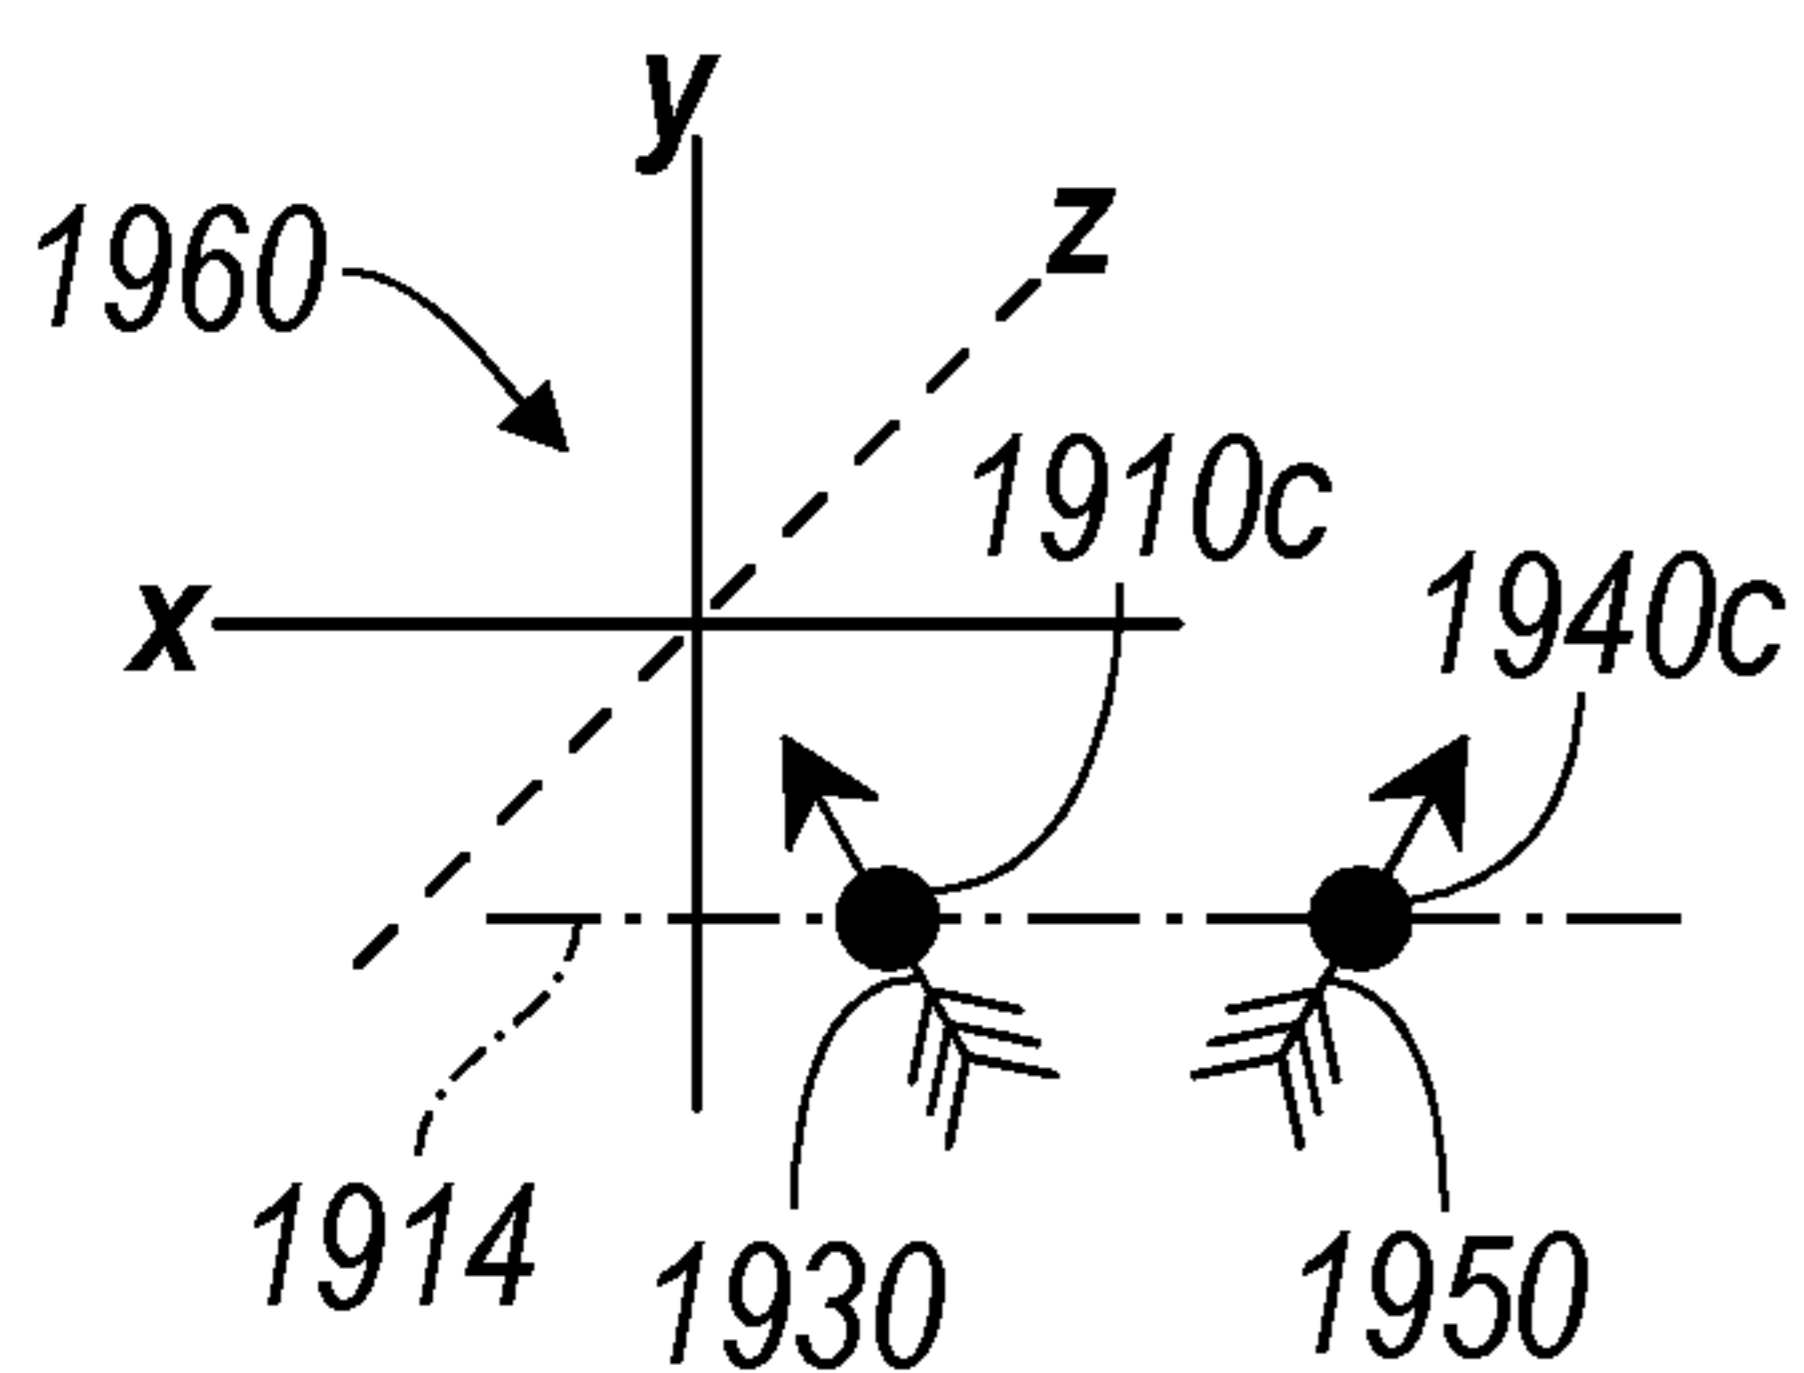


FIG. 86A

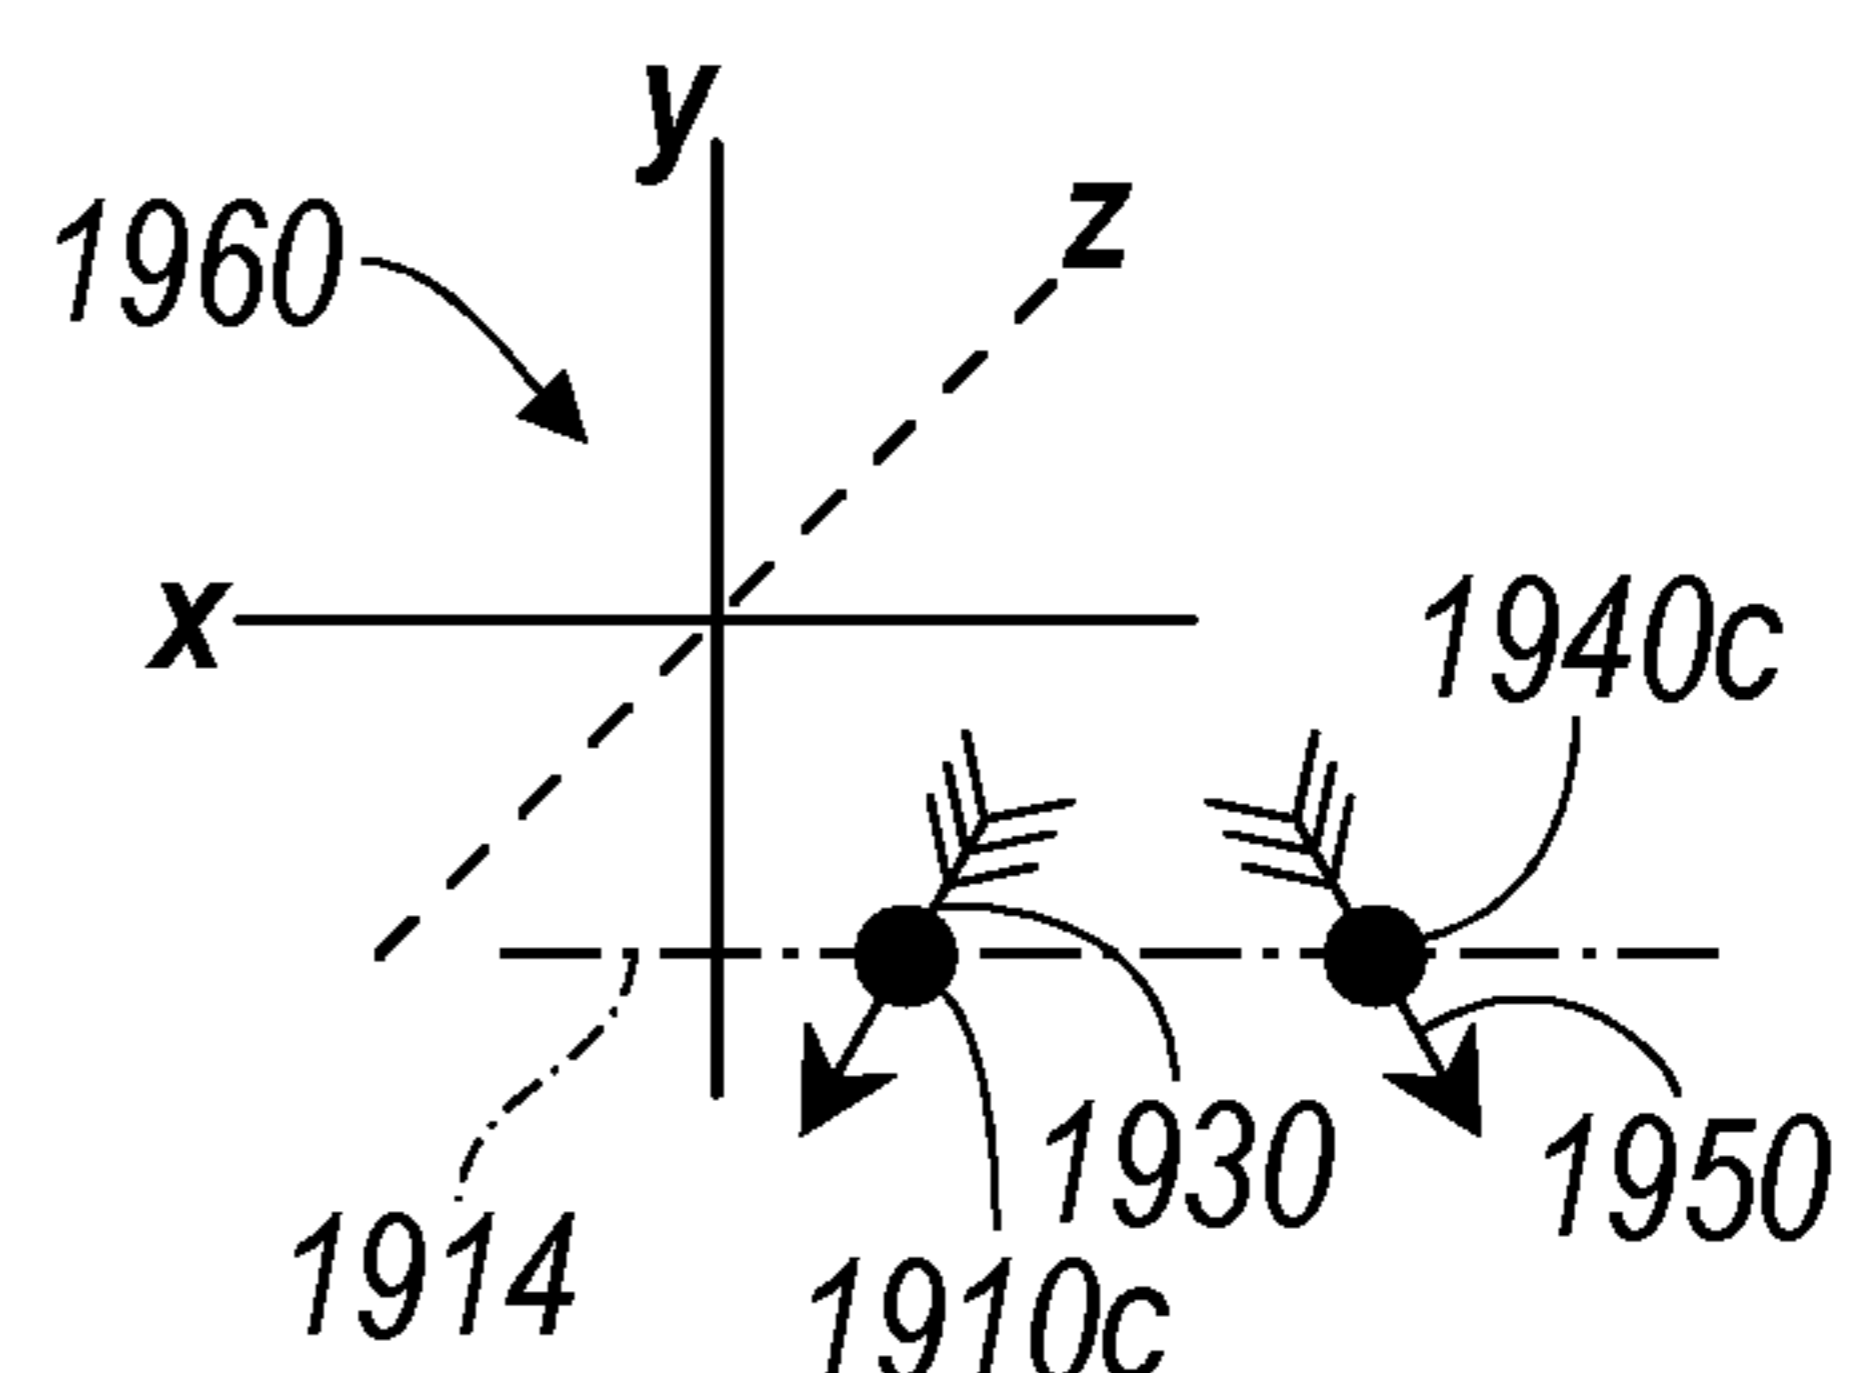


FIG. 86B

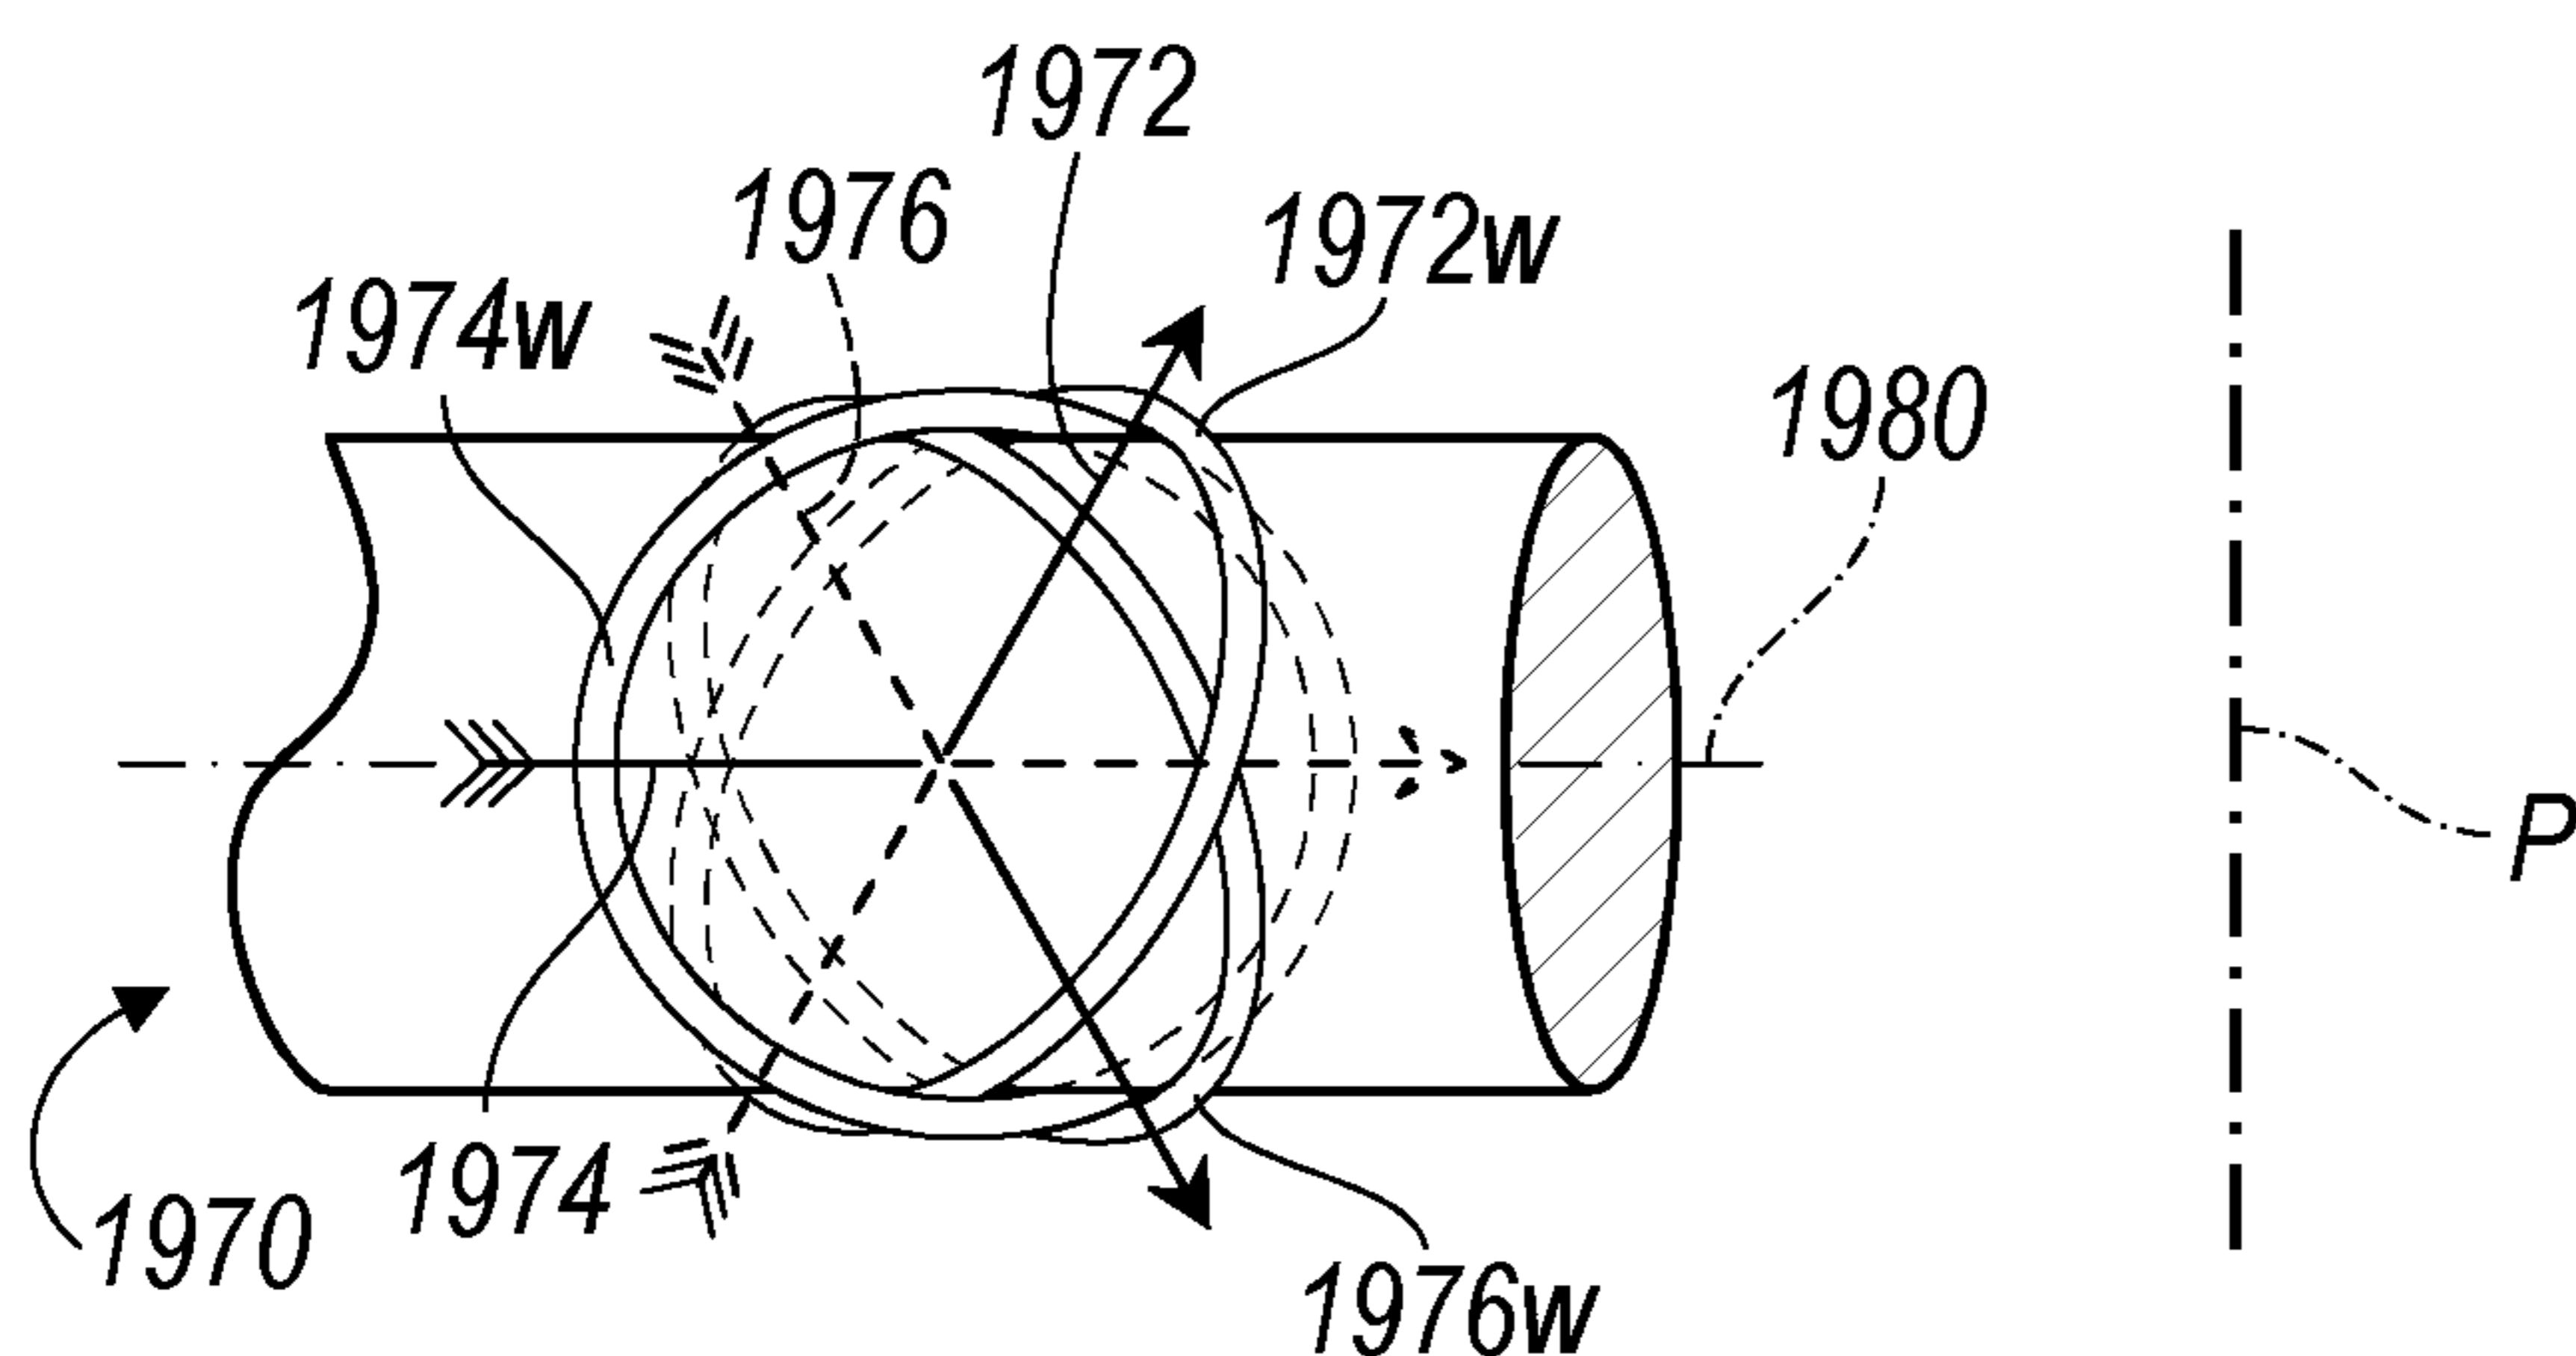


FIG. 87A

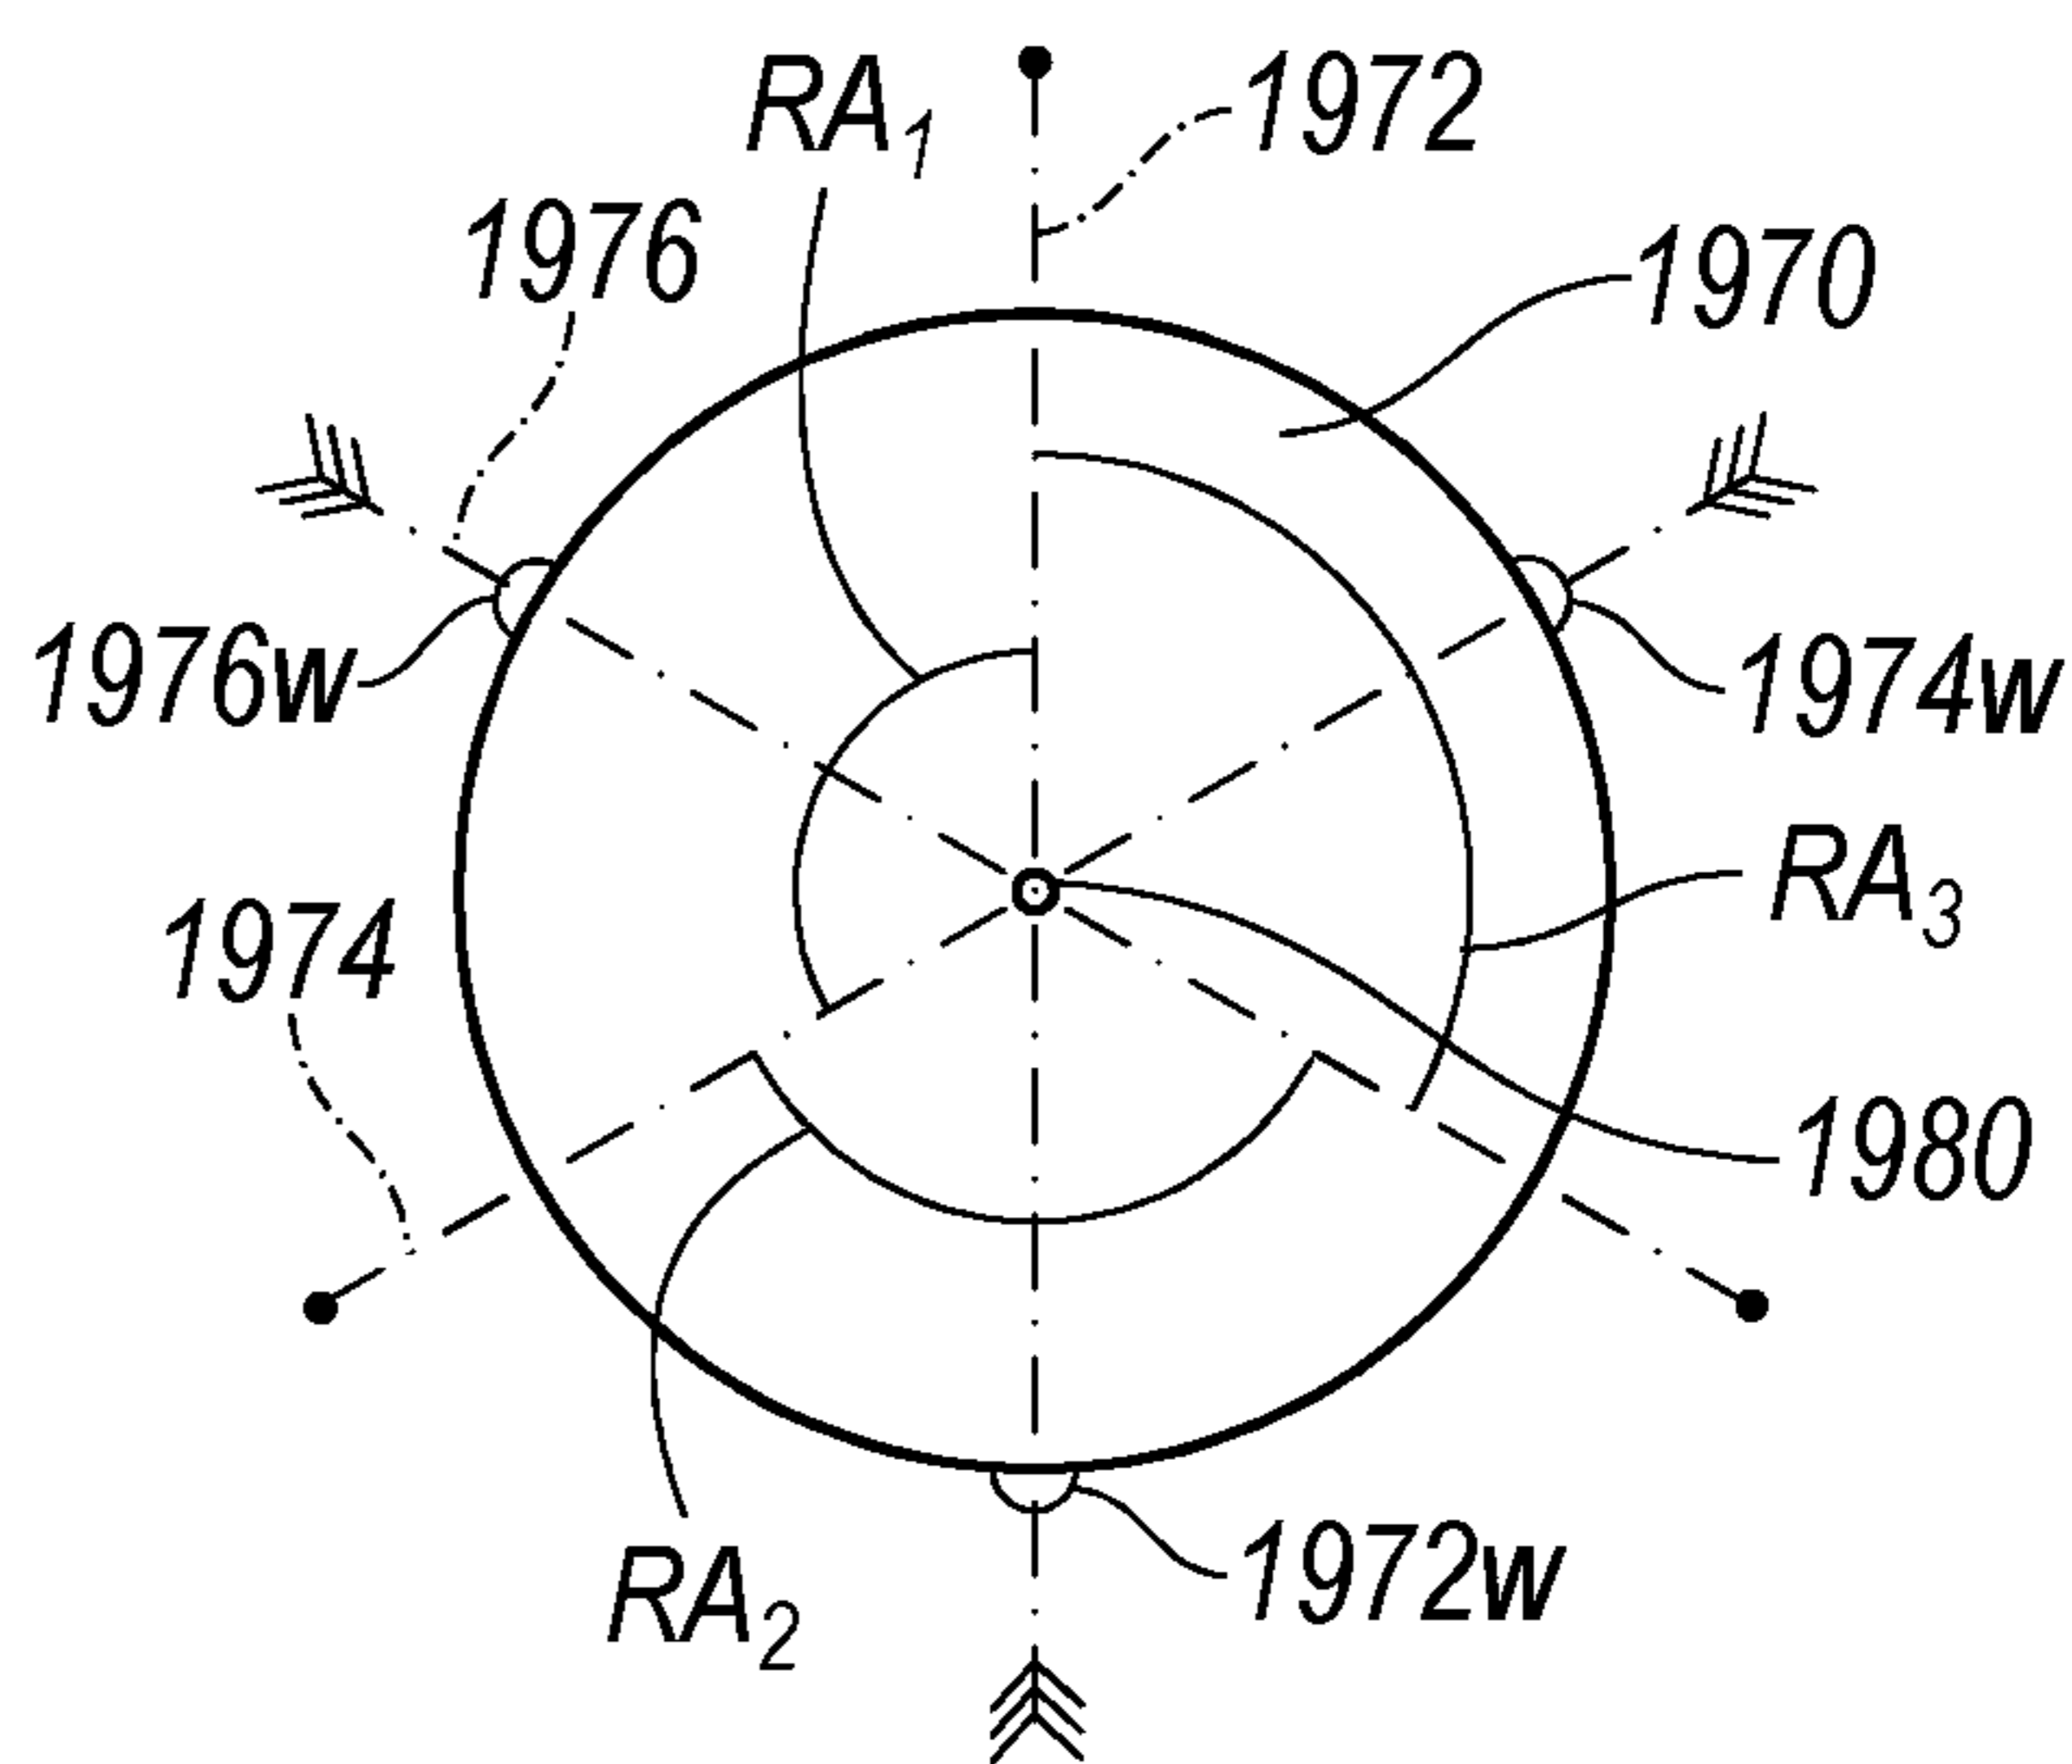


FIG. 87B

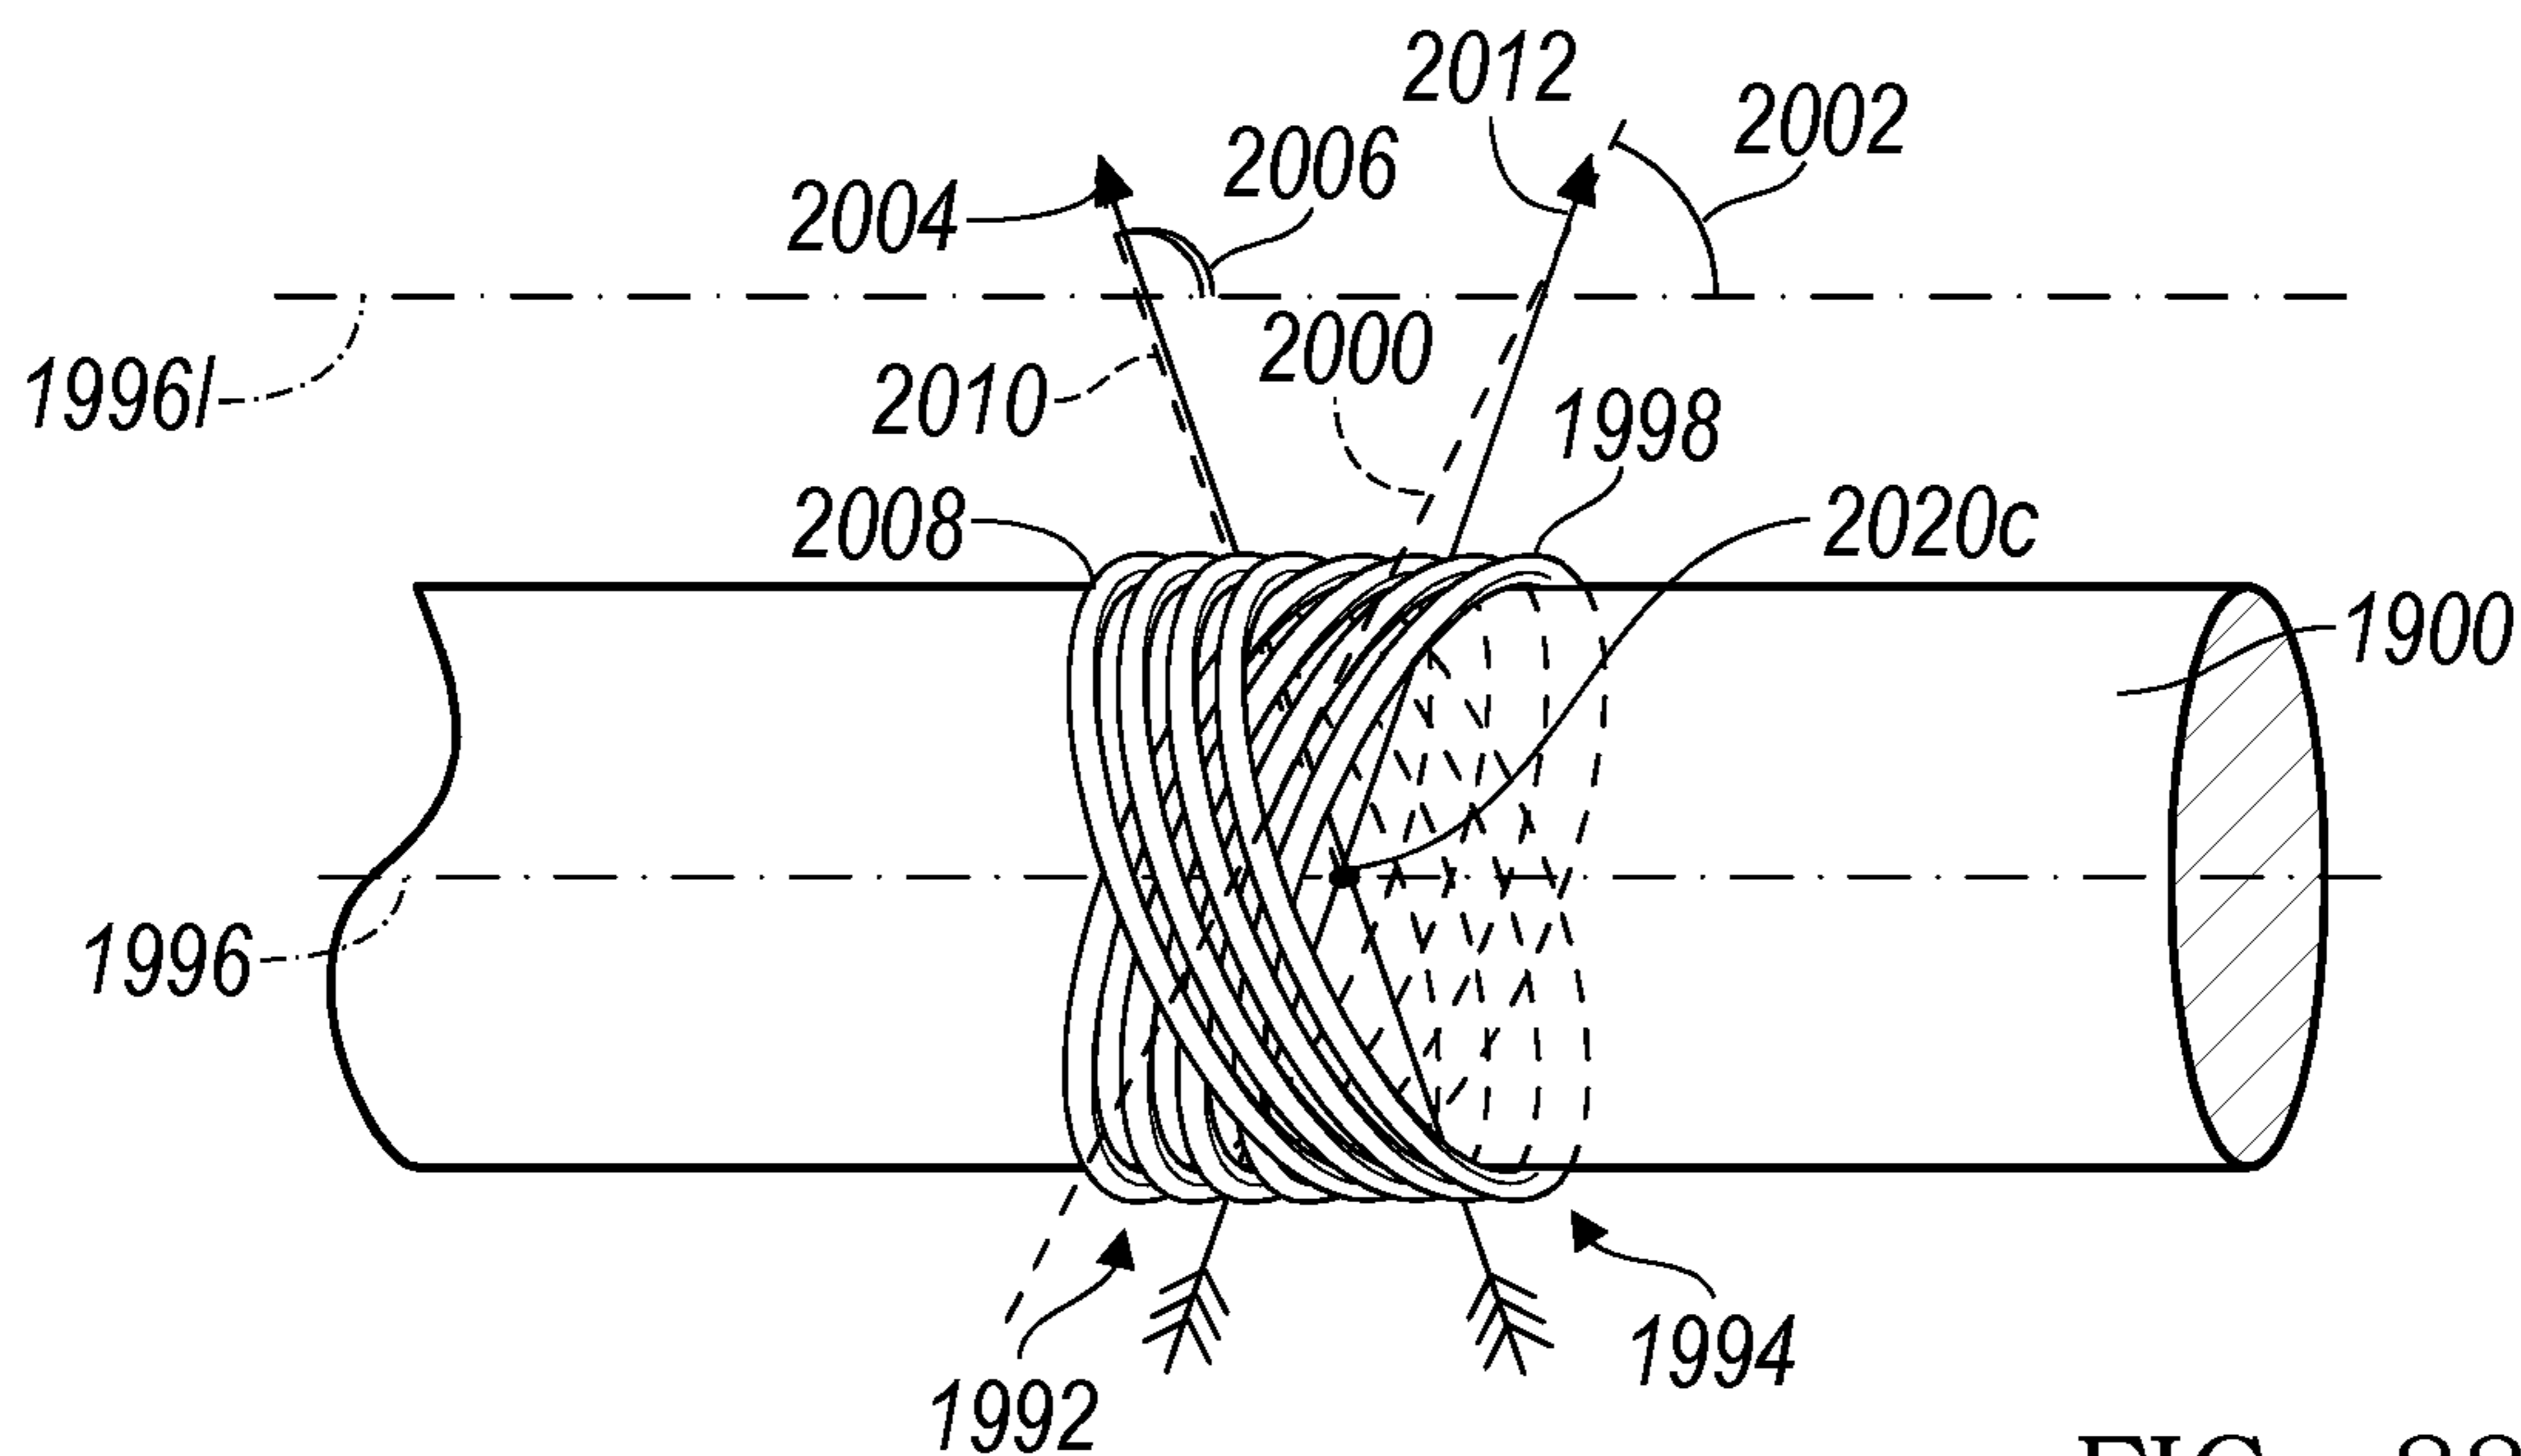


FIG. 88

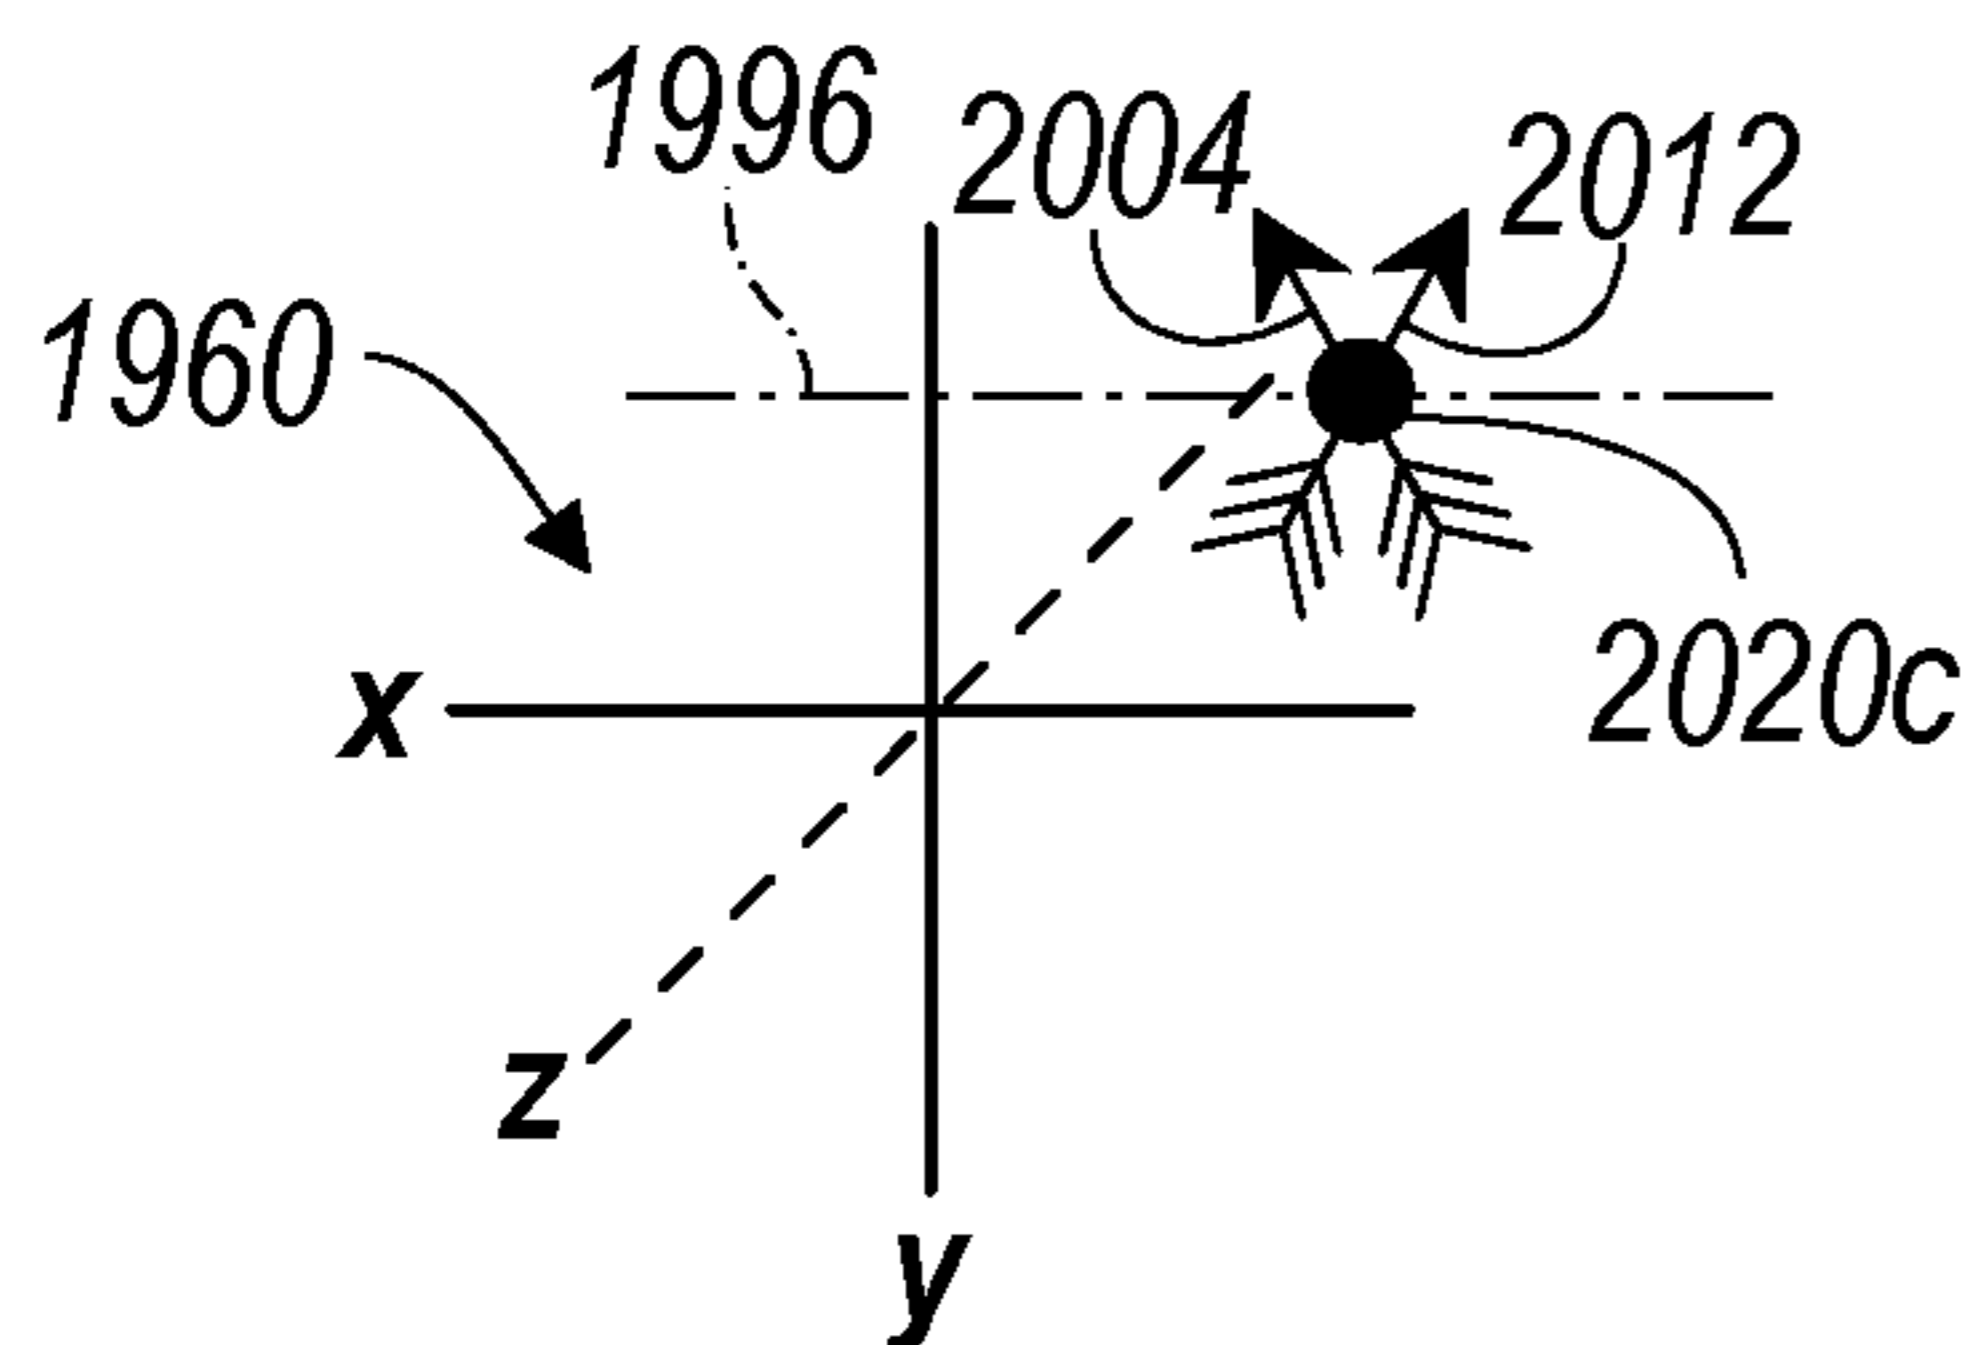


FIG. 89A

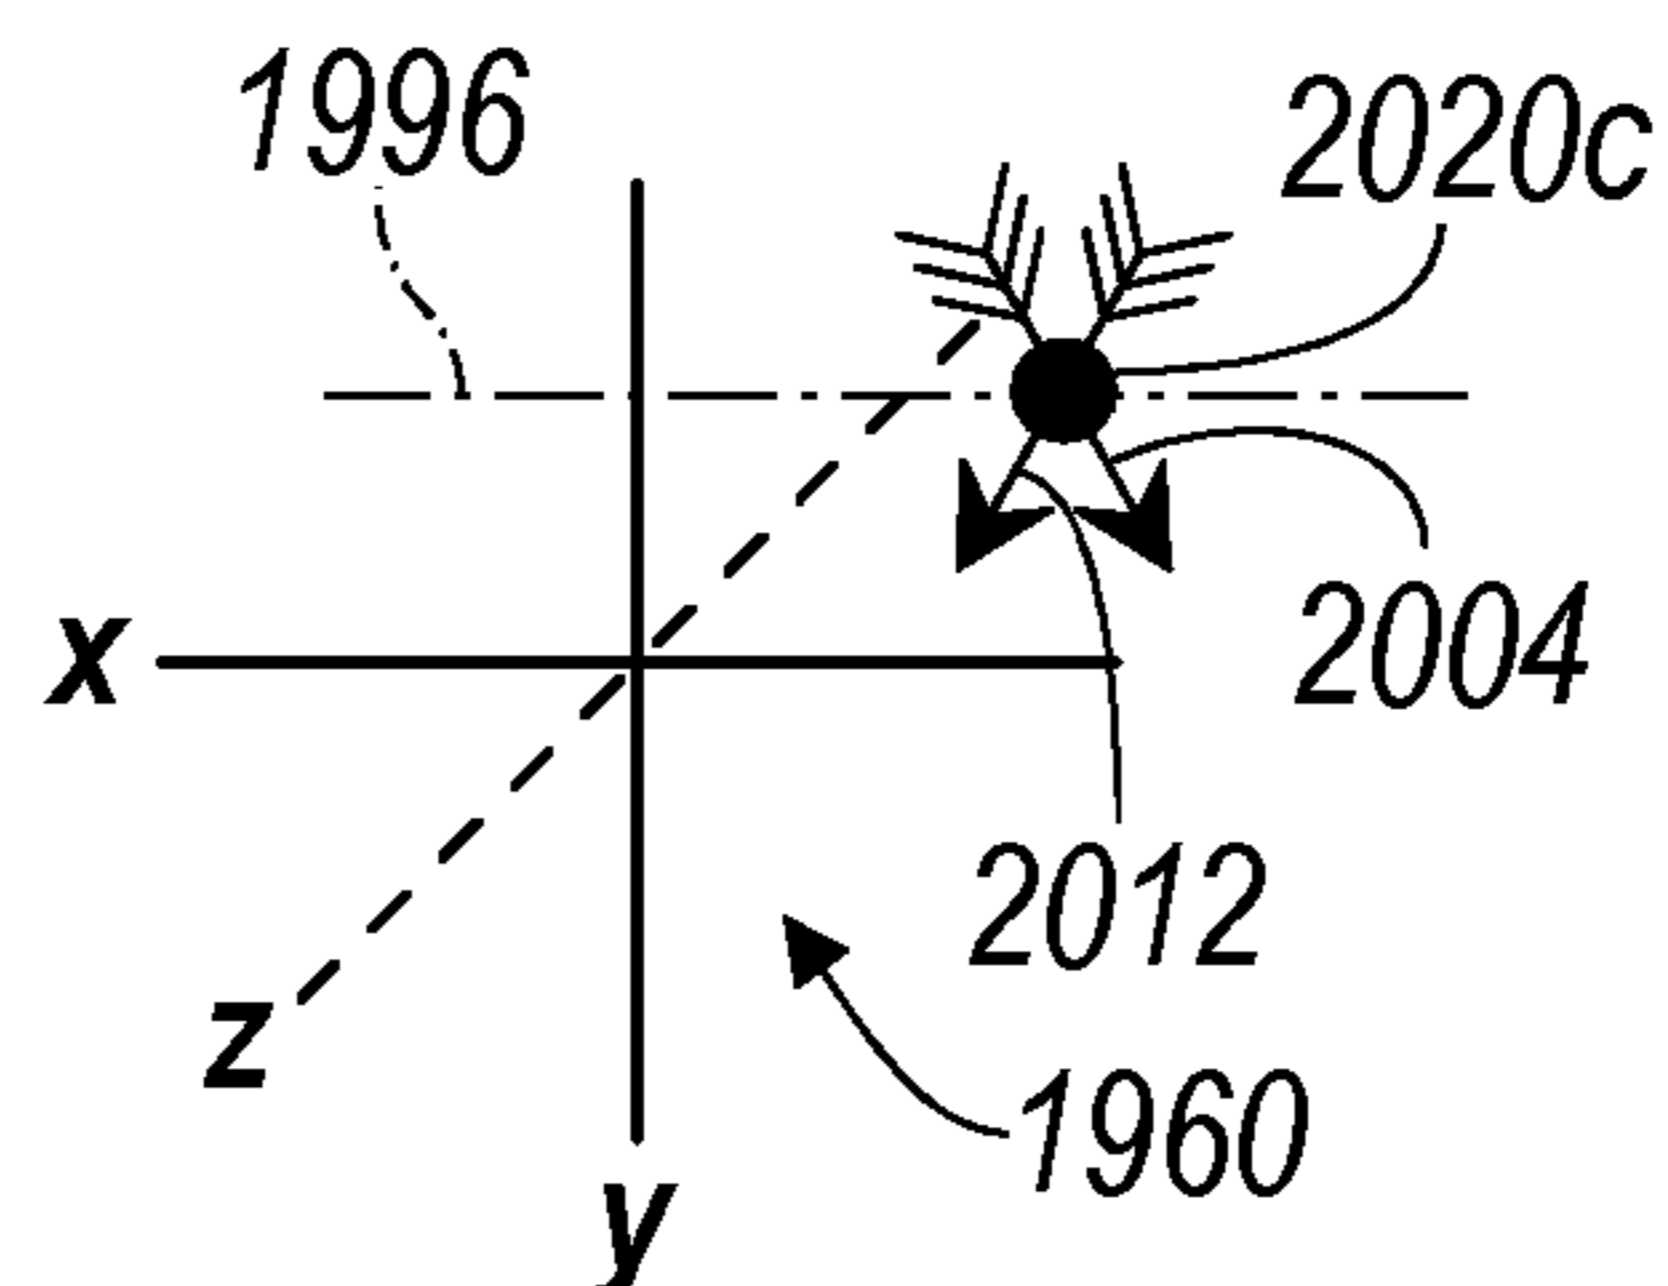


FIG. 89B

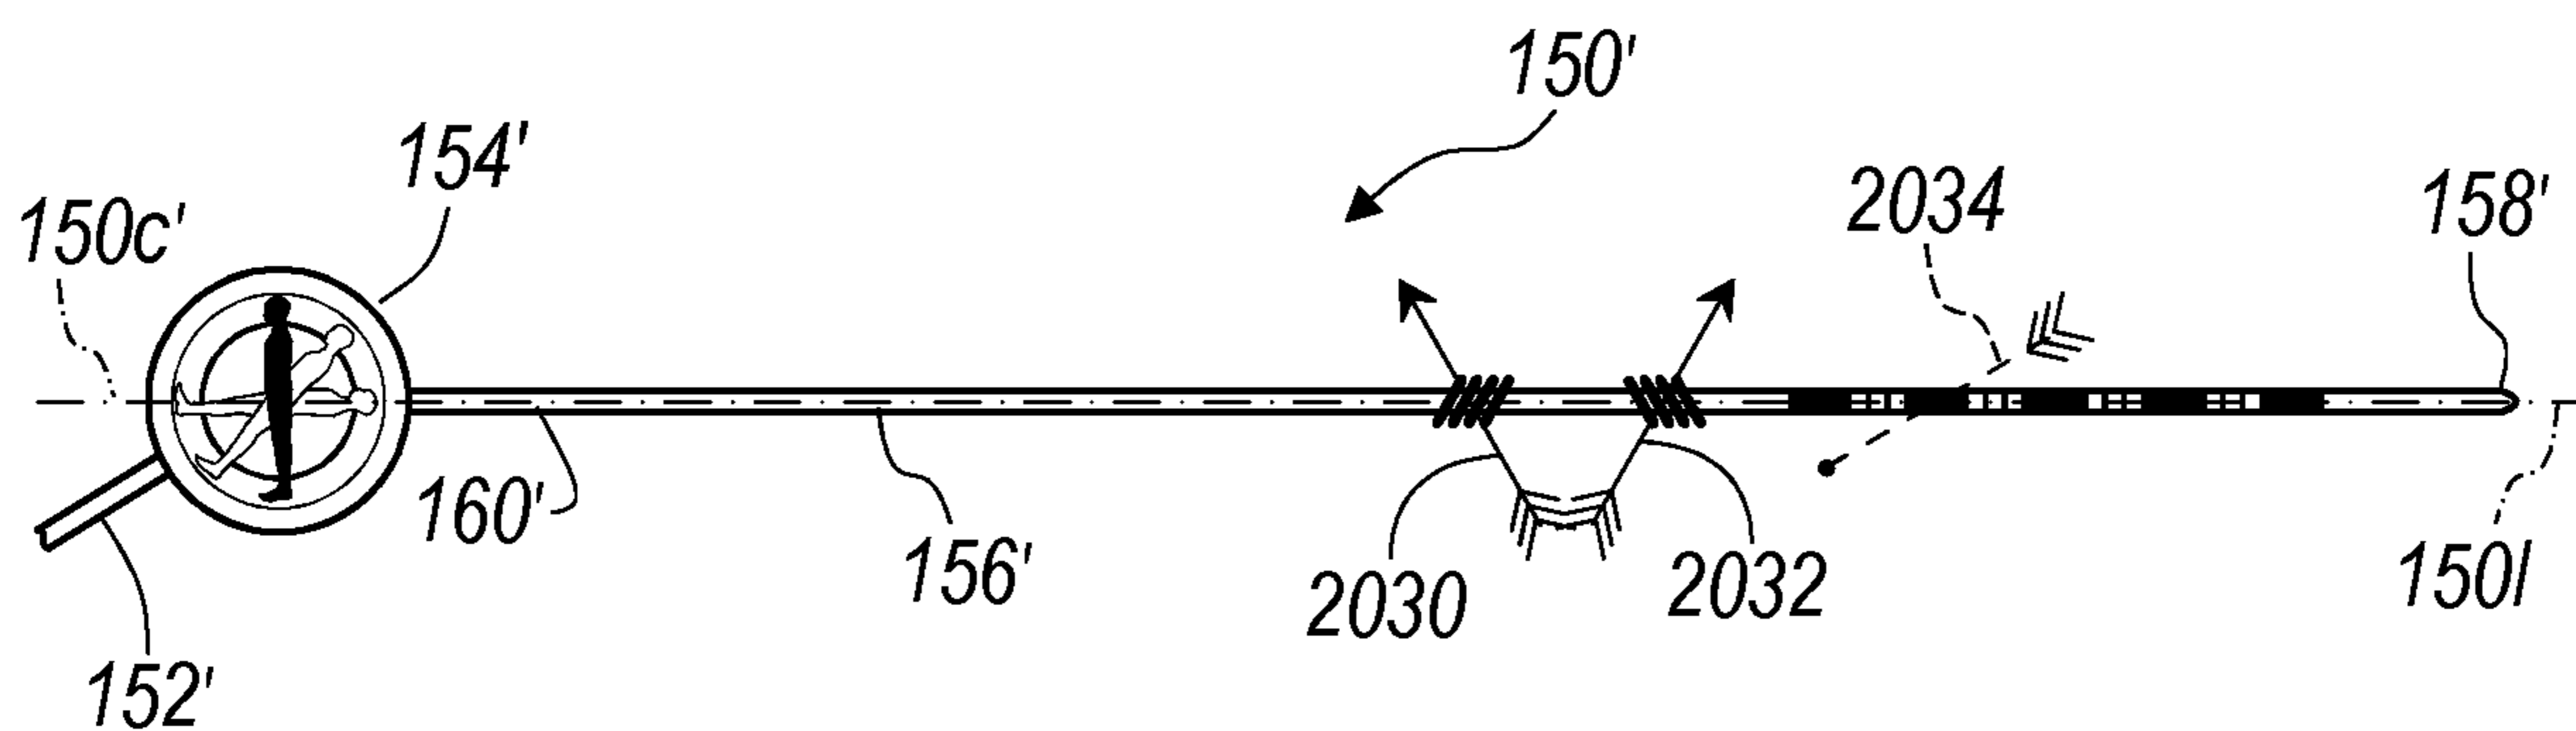


FIG. 90

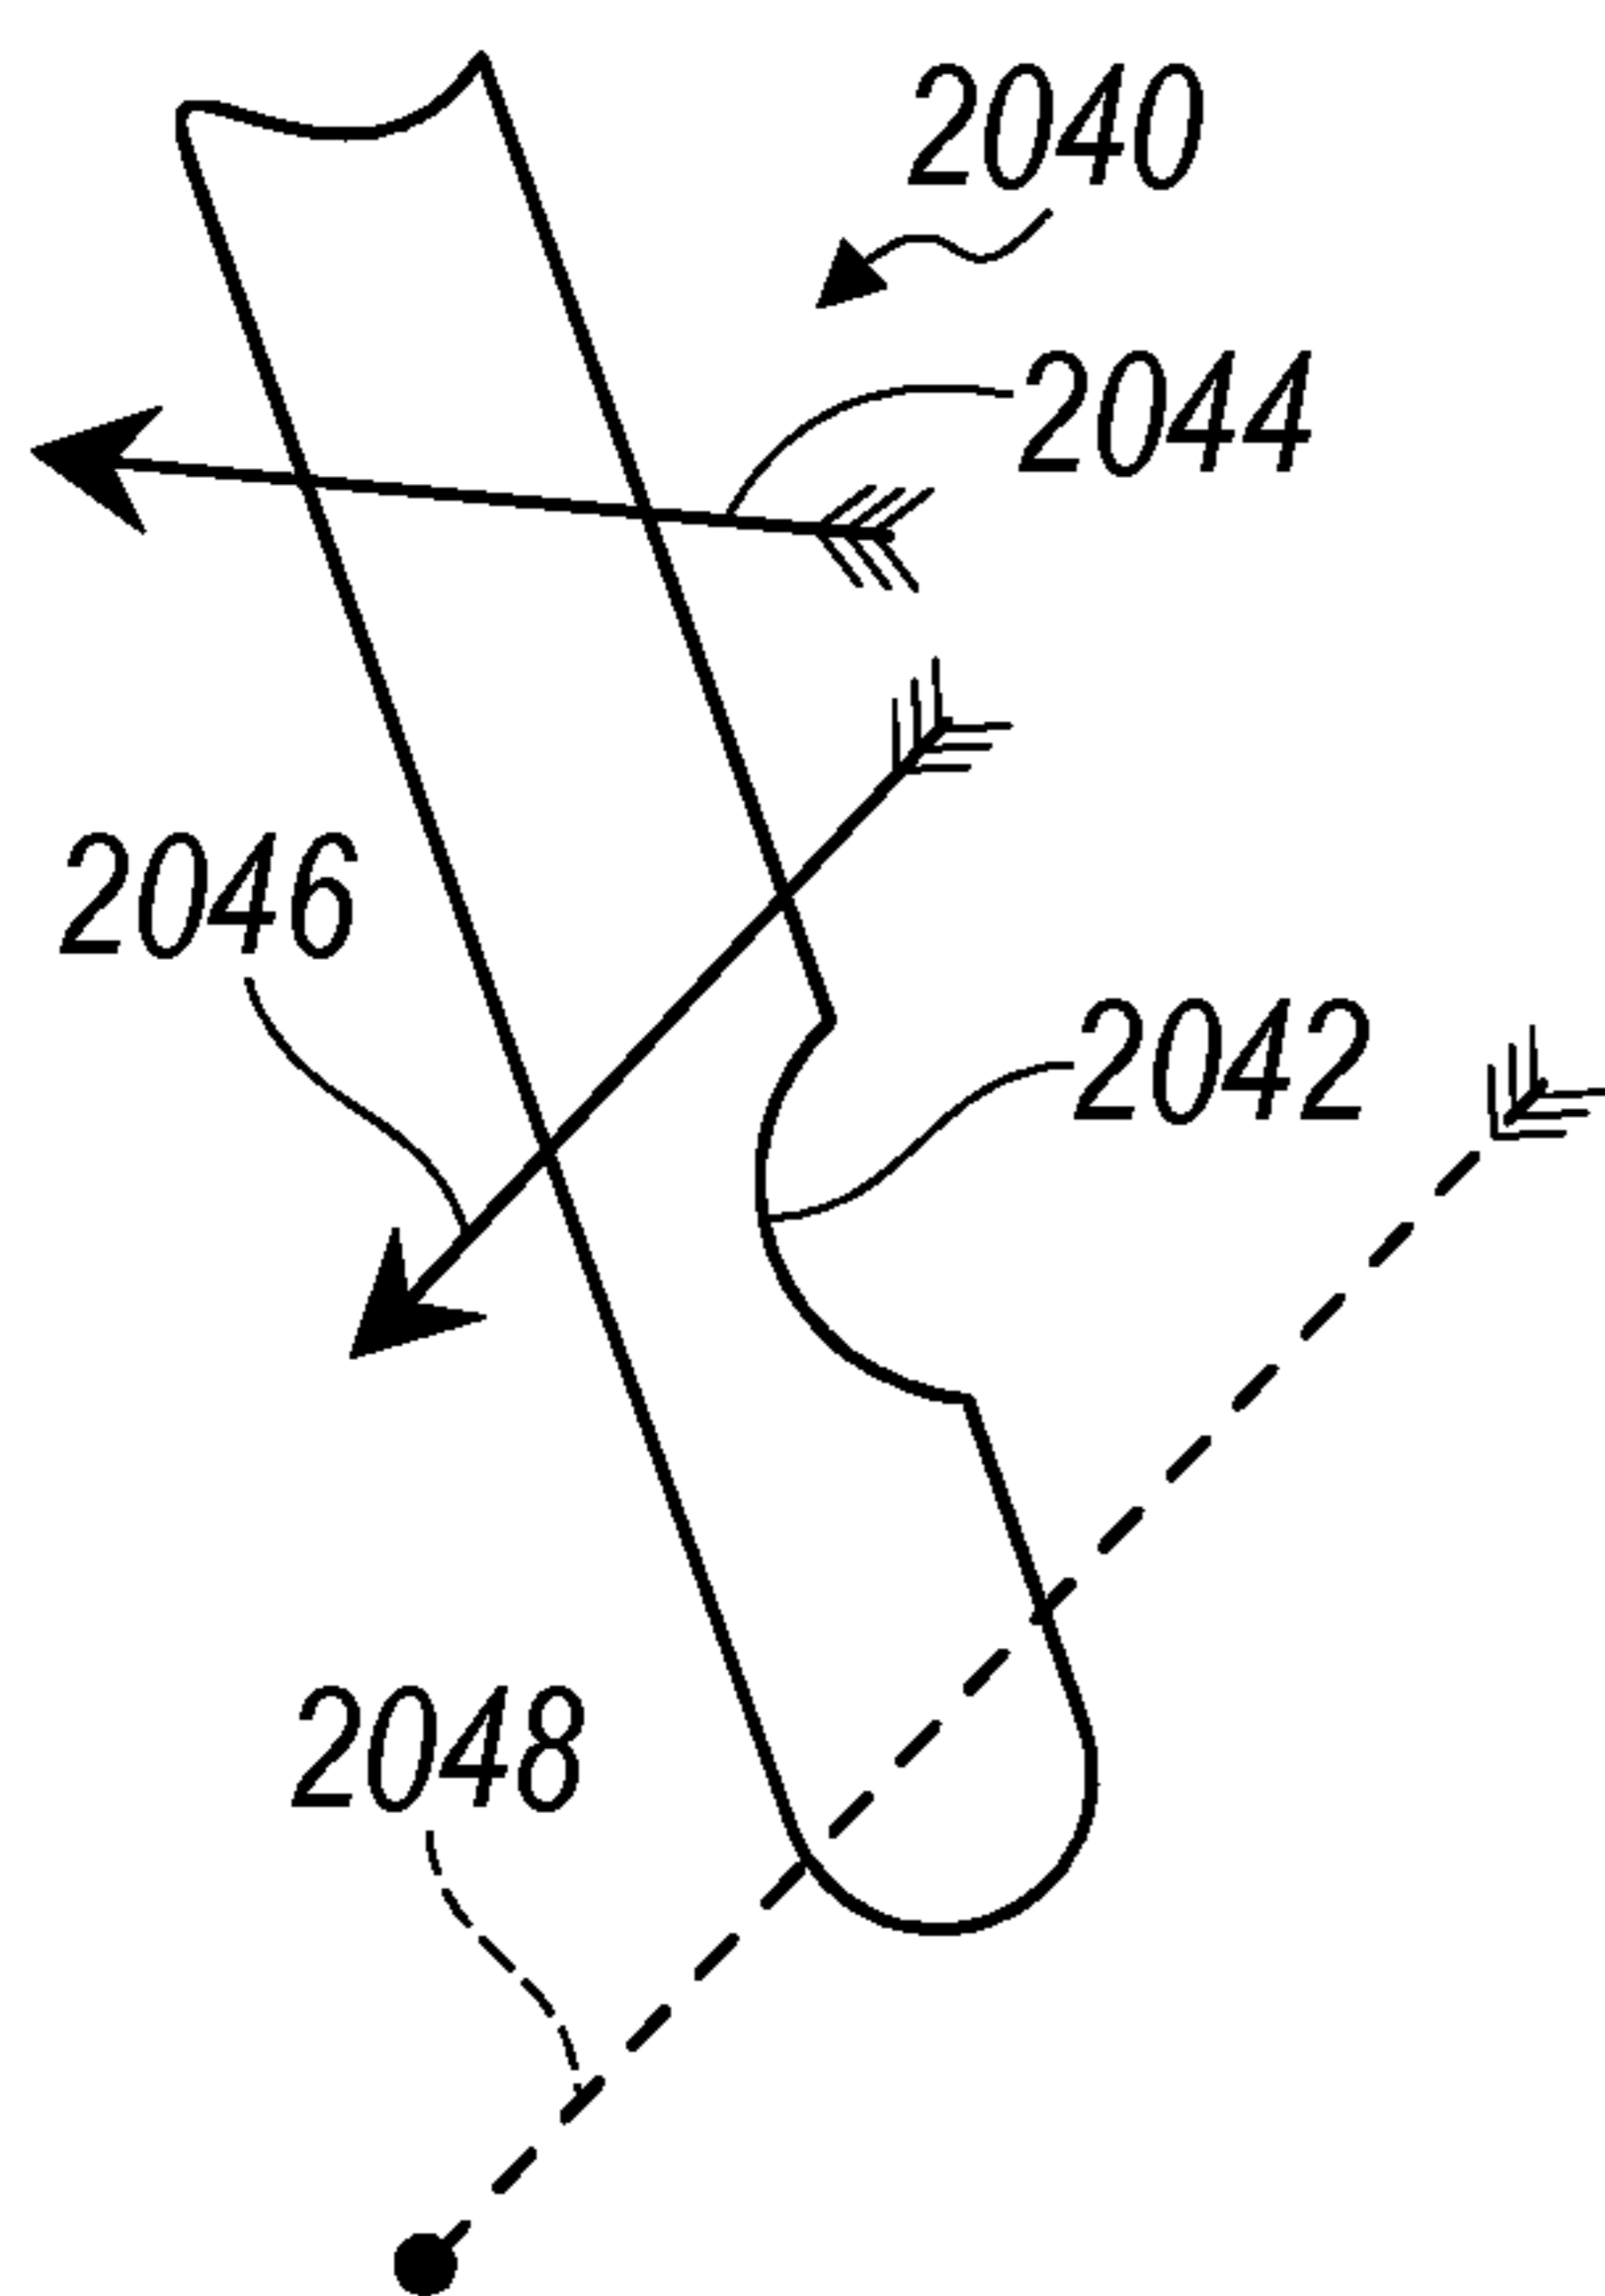


FIG. 91A

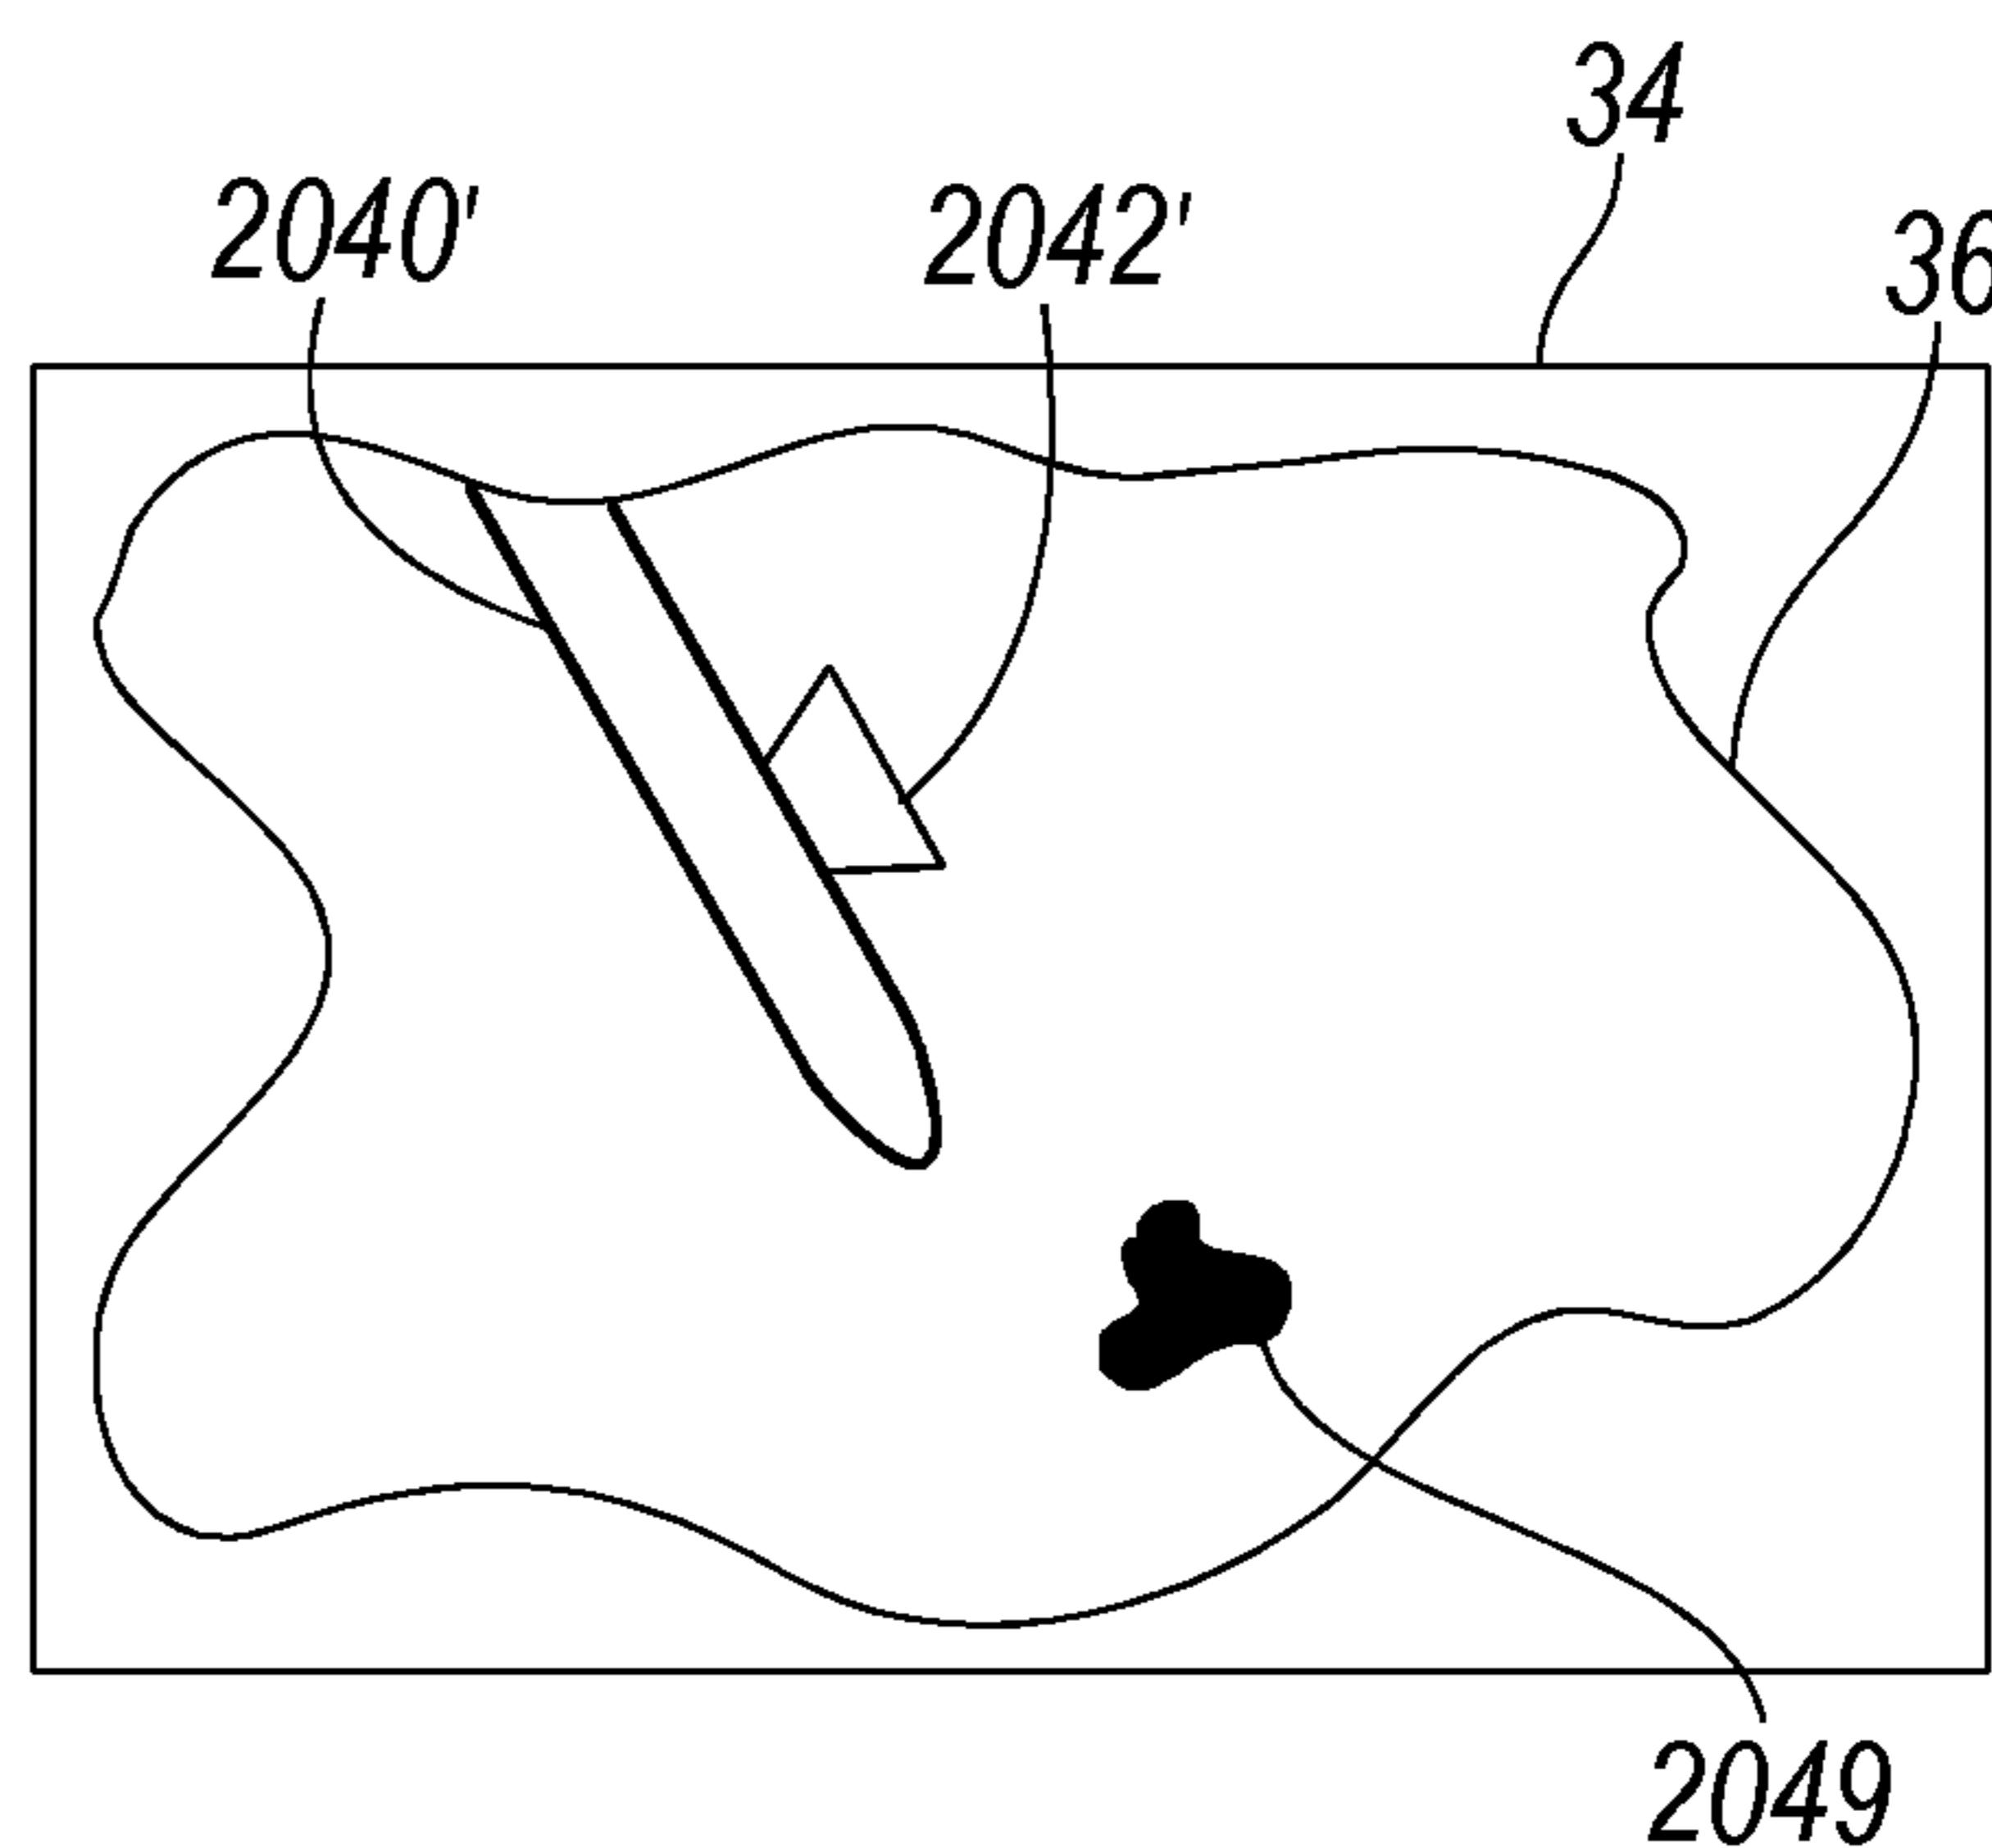


FIG. 91B

FIG. 92

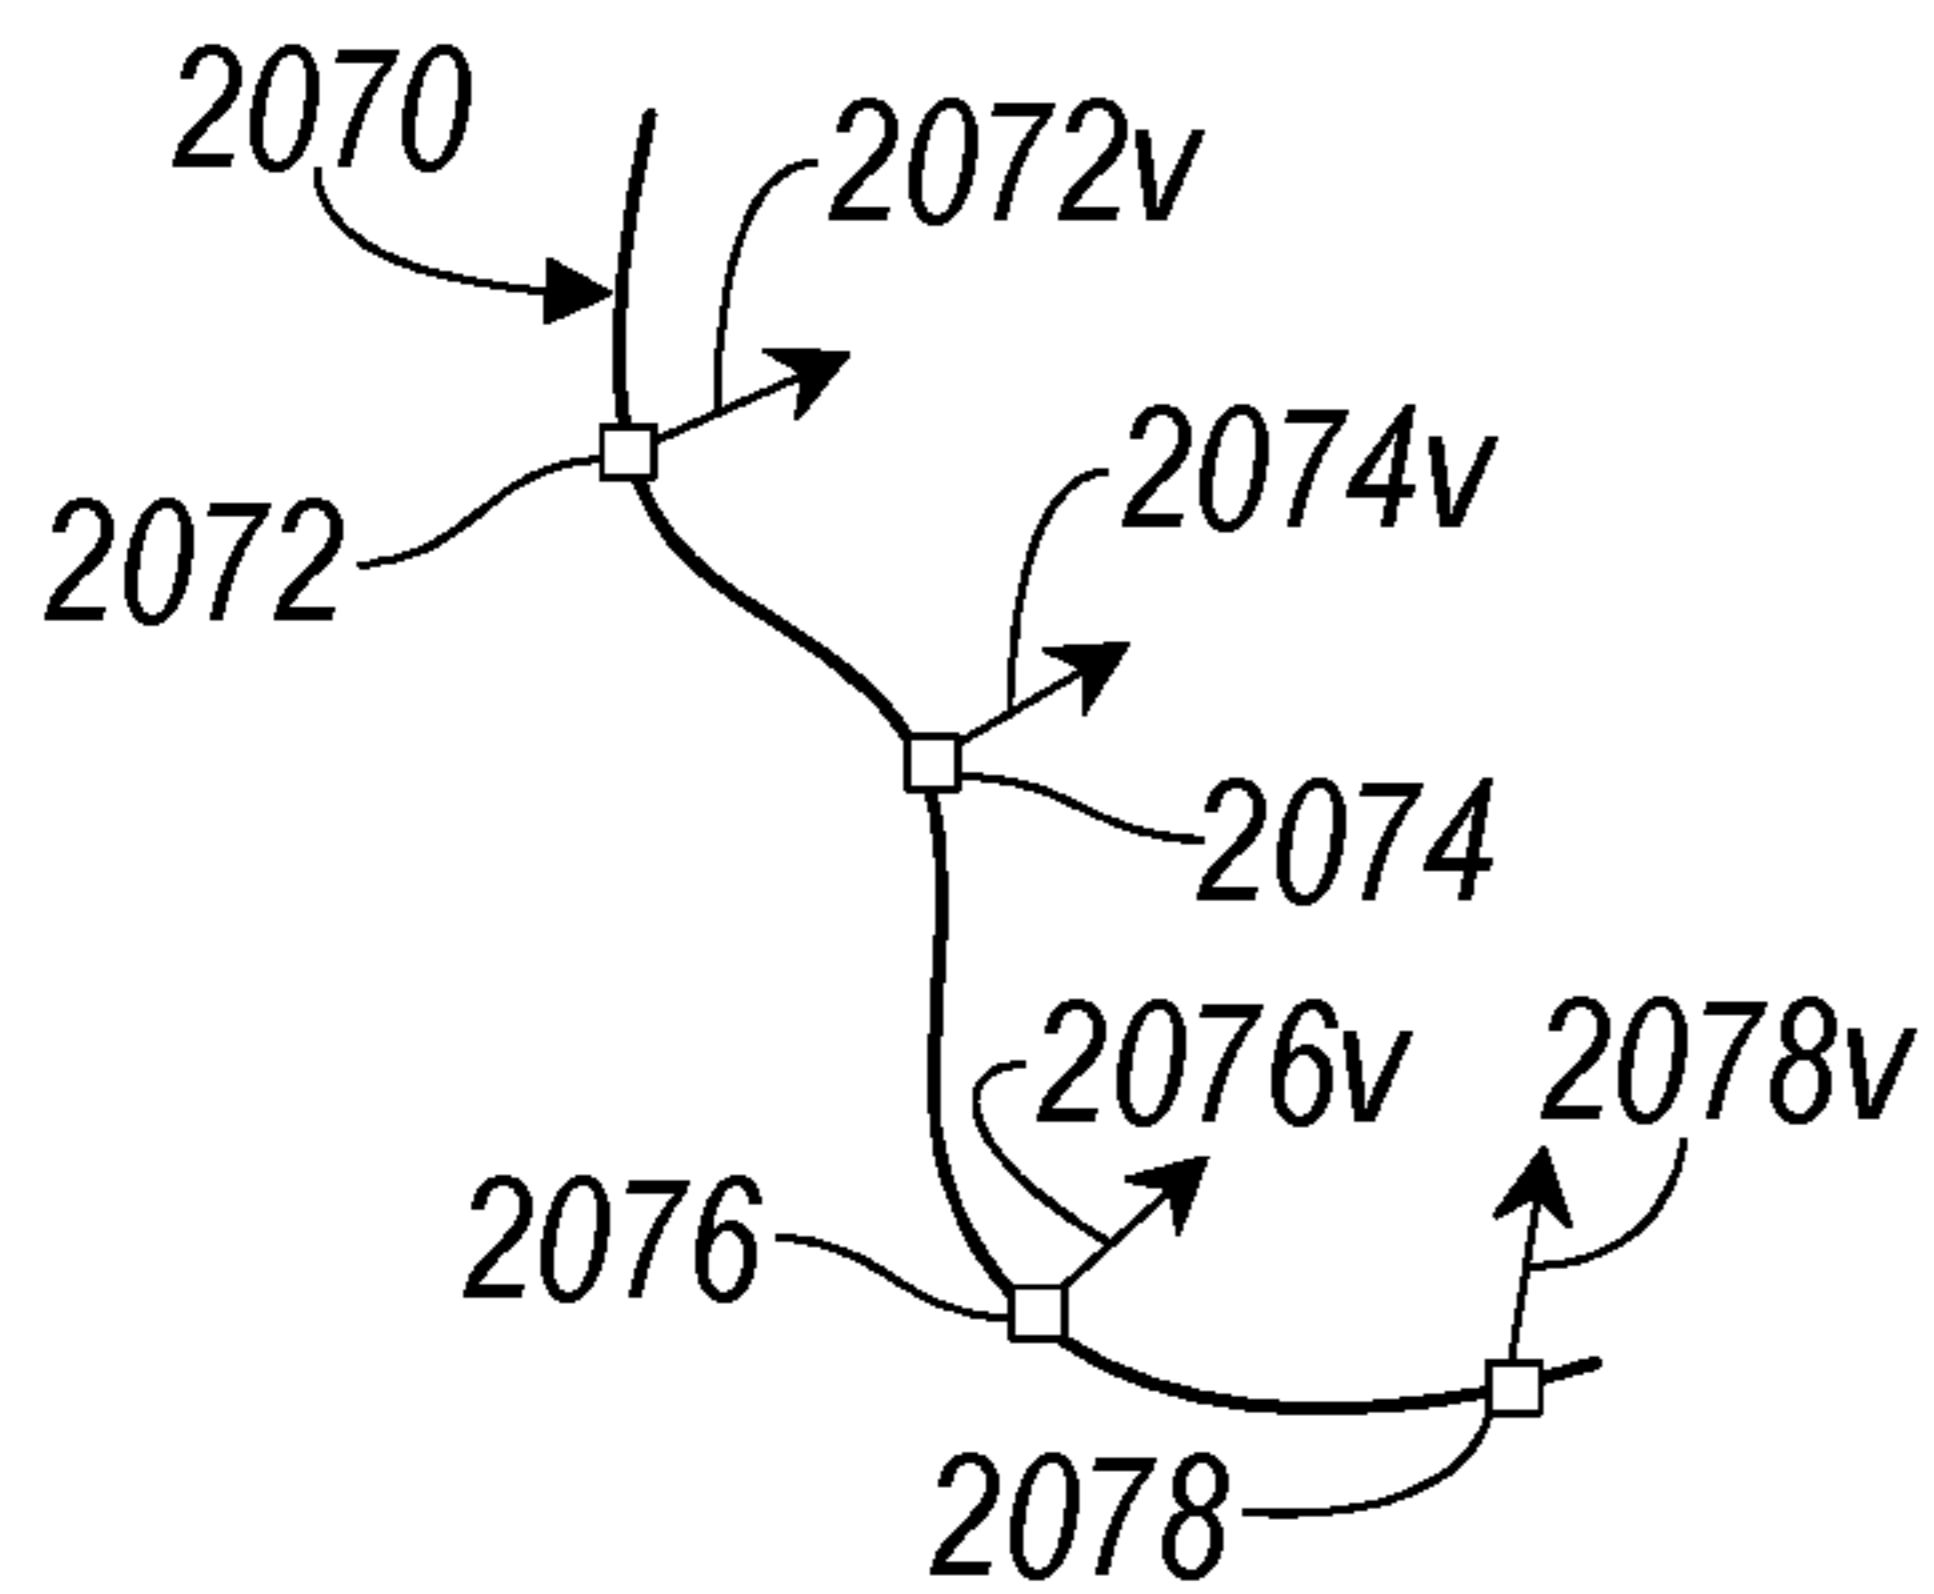
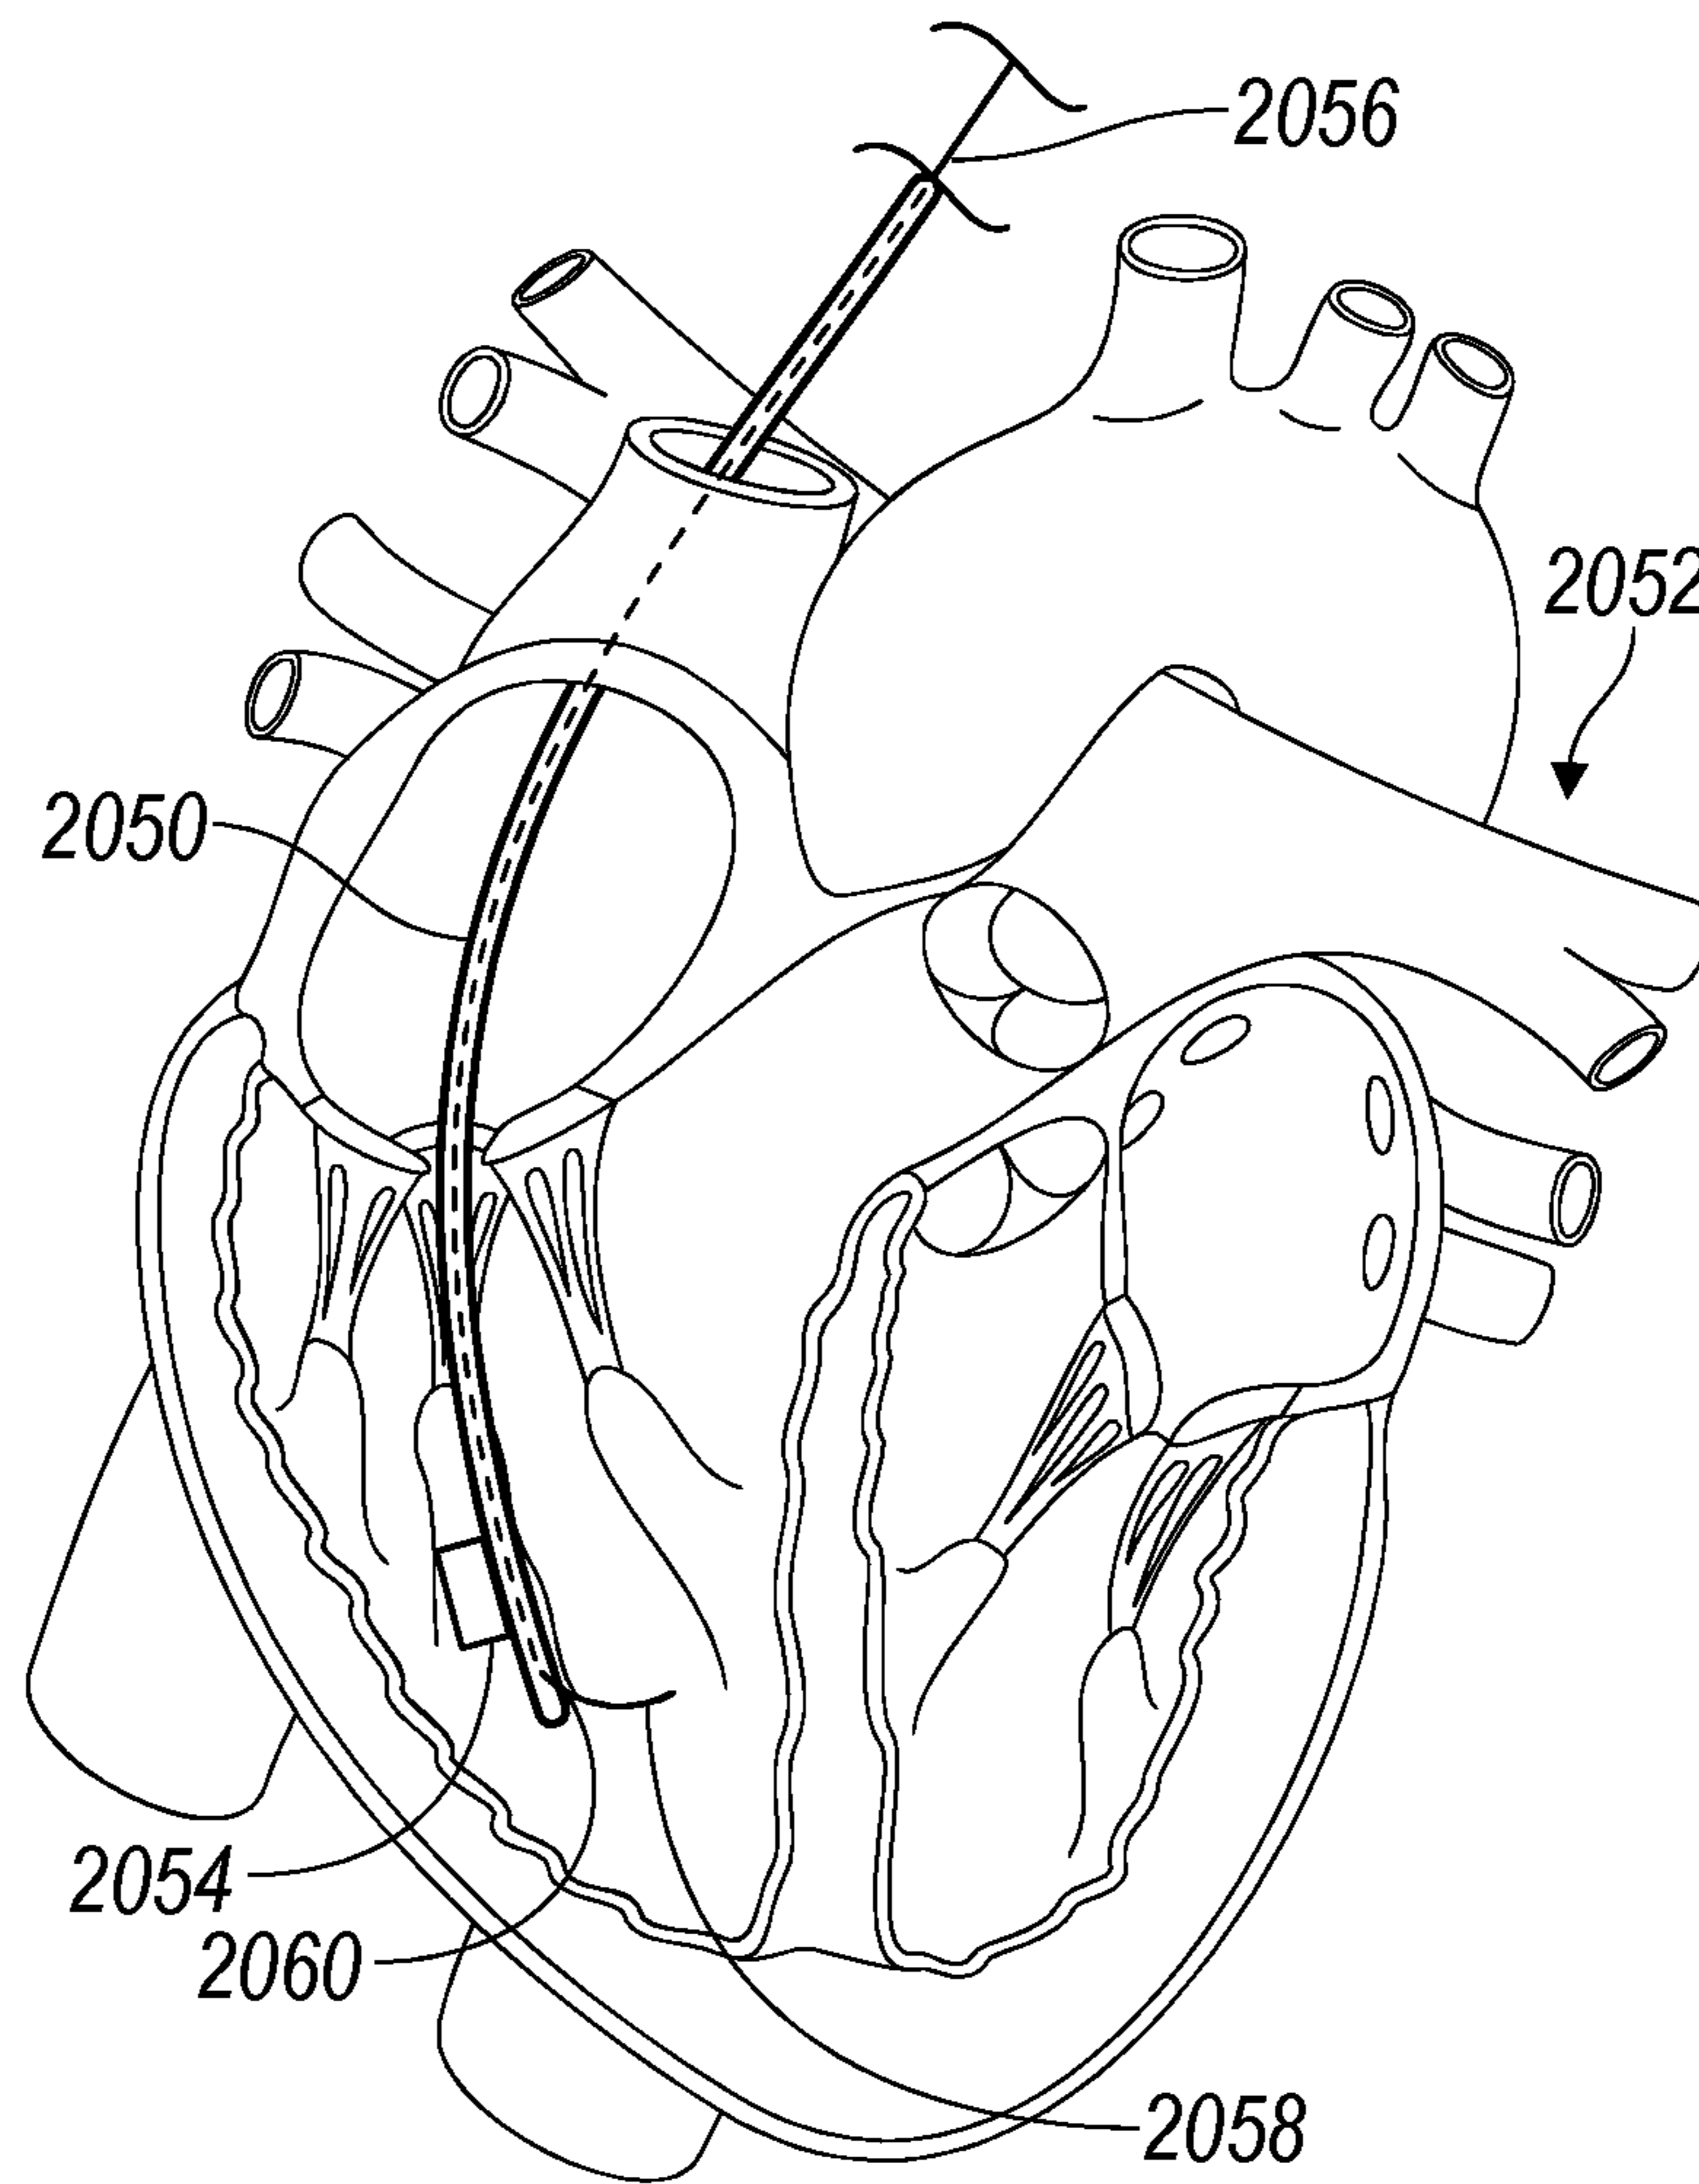


FIG. 93A

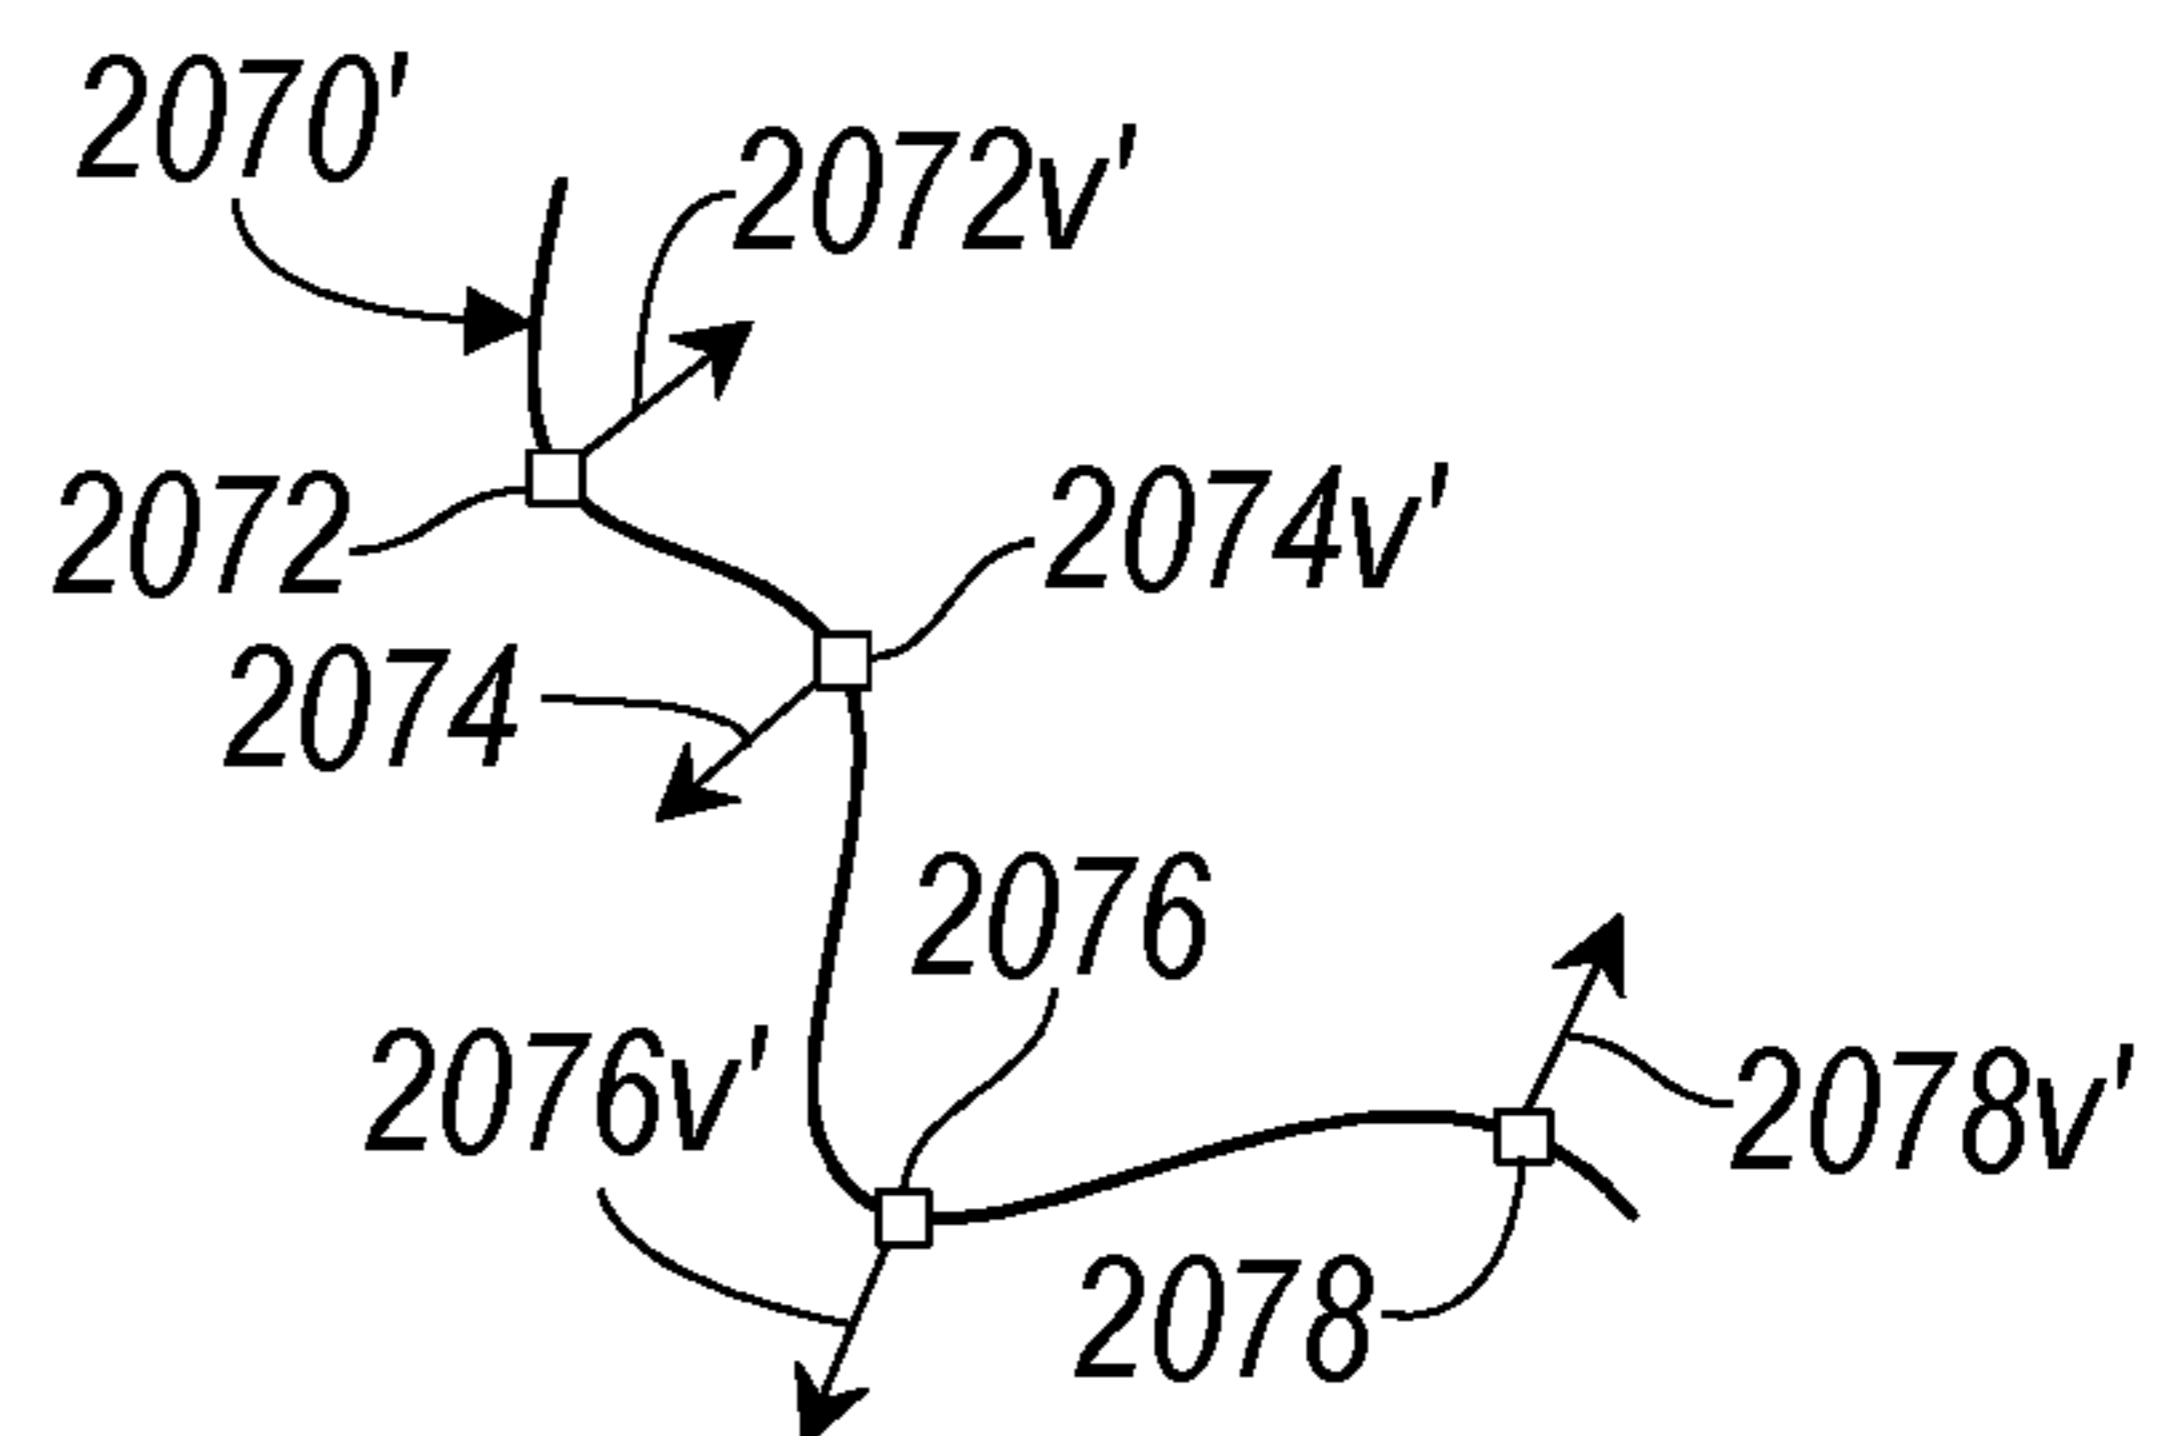


FIG. 93B

METHOD AND APPARATUS FOR SURGICAL NAVIGATION

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 14/171,346 filed on Feb. 3, 2014, which is a continuation of U.S. patent application Ser. No. 12/770,181 filed on Apr. 29, 2010, now U.S. Pat. No. 8,644,907 issued on Feb. 4, 2014, which is a continuation-in-part of U.S. patent application Ser. No. 11/247,848 filed on Oct. 11, 2005, now U.S. Pat. No. 8,057,407 issued on Nov. 15, 2011, which is a continuation of U.S. patent application Ser. No. 10/289,869 filed on Nov. 7, 2002, now U.S. Pat. No. 7,007,699 issued on Mar. 7, 2006, which is a continuation of U.S. patent application Ser. No. 09/428,721 filed on Oct. 28, 1999, now U.S. Pat. No. 6,499,488 issued on Dec. 31, 2002. The disclosures of the above applications are incorporated herein by reference.

This application is a continuation of U.S. patent application Ser. No. 14/171,346 filed on Feb. 3, 2014, which is a continuation of U.S. patent application Ser. No. 12/770,181 filed on Apr. 29, 2010, now U.S. Pat. No. 8,644,907 issued on Feb. 4, 2014, which is also a continuation-in-part of U.S. patent application Ser. No. 11/179,044 filed on Jul. 11, 2005, now U.S. Pat. No. 8,239,001 issued on Aug. 7, 2012, which is a continuation-in-part of U.S. patent application Ser. No. 10/941,782 filed on Sep. 15, 2005, now U.S. Pat. No. 7,751,865 issued on Jul. 6, 2010, which is a continuation-in-part of U.S. patent application Ser. No. 10/688,068 filed on Oct. 17, 2003, now U.S. Pat. No. 7,366,562 issued on Apr. 29, 2008. The disclosures of the above applications are incorporated herein by reference.

FIELD

The present teachings relate generally to navigated surgery, and more specifically, to systems and methods for using instruments and systems to assist in navigating surgical procedures in internal body structures.

BACKGROUND

Image guided medical and surgical procedures utilize patient images obtained prior to or during a medical procedure to guide a physician performing the procedure. Recent advances in imaging technology, especially in imaging technologies that produce highly-detailed, two, three, and four dimensional images, such as computed tomography (CT), magnetic resonance imaging (MRI), fluoroscopic imaging (such as with a C-arm device), positron emission tomography (PET), and ultrasound imaging (US) has increased the interest in image guided medical procedures.

Typical image guided navigation systems generally require dynamic reference frames to track the position of the patient should patient movement occur during the assisted procedure. The dynamic reference frame is generally affixed to the patient in a generally permanent or immovable fashion. The dynamic reference frame may also be used as a fiducial marker and may, therefore, be attached to the patient during the acquisition of pre-operative images. This enables the image space to be aligned with patient space during the navigated procedure. For example, with relation to a cranial procedure, the dynamic reference frame can be attached to the skull by a bone screw. For other procedures the dynamic reference frame may be fixed to other bony

portions also with bone screws. Regardless, the dynamic reference frame may include a portion that is fixed to the patient during the acquisition of the pre-operative images and remains attached until the procedure is complete to insure proper and accurate correlation between image space and patient space. Requiring that the dynamic reference frame be attached to the patient during the time that the pre-acquired images are acquired until the procedure actually takes place may be uncomfortable.

The dynamic reference frame may, then be used to assure that images of a patient, such as pre-acquired or atlas images, may be registered to the patient space. Generally this registration also allows for tracking of various instruments during a procedure. The tracked instruments will generally include portions that may be tracked and superimposed over acquired or modeled images of the patient.

Various instruments may be used during an operative procedure that are desired to be tracked. Even if images are acquired, either intra-operatively or pre-operatively, the instrument is generally illustrated, and superimposed on the captured image data to identify the position of the instrument relative to the patient space. Therefore, the instrument may include detectable portions, such as electromagnetic coils or optical detection points, such as LEDs or reflectors, that may be detected by a suitable navigation system.

Size considerations generally make it difficult to position the tracking sensors near a portion of the instrument to be positioned within the patient, such as the distal tip. Because of this, the tracking sensors are generally positioned within the handle of the instrument. Therefore, complex calculations and a degree of error may exist to determine the exact position of a distal end of the instrument relative to the position of the detectable sensors. Also the instruments may flex unexpectedly so that the known dimensions are no longer true dimensions of the instrument. Therefore, it may be desirable to provide sensors substantially near the distal tip or end of an instrument positioned within a patient.

The tracking of various sensor portions, such as electromagnetic coils, may require the transmission of a current or a voltage to or from the sensors. Therefore, an electrical potential is provided to an instrument that is often positioned within a portion of the patient's anatomy, which may include various portions such as the cardiac area, neurological area, and other areas of the patient. In order to provide separation of these potentials from the patient, it may also be desirable to isolate the potentials from the patient.

SUMMARY

An instrument can be tracked during a procedure, such as a surgical procedure. The instrument, because it is tracked, can be illustrated on a display device with image data for illustrating the location of the instrument. The location of the instrument can include both its 3-dimensional position (x,y,z) and its 3 degrees of orientation (yaw, pitch, and roll). These six variables can provide 6 degree of freedom information regarding the position and orientation (herein referred together as location) of the instrument. This can be achieved by providing one or more tracking devices on a long instrument wherein the navigated orientation of the tracking device is at an angle to the shaft around which it is round, which is also at an angle to the tracking device's long axis.

A surgical navigation system for navigating a region of a patient includes a non-invasive dynamic reference frame and/or fiducial marker, sensor tipped instruments, and isolator circuits. The dynamic reference frame may be repeat-

ably placed on the patient in a non-invasive manner and in a precise location for guiding the instruments. The instruments may be precisely guided by positioning sensors near moveable portions of the instruments. The patient may be electrically isolated from various sources of current during the procedure.

According to various embodiments a surgical navigation system includes a method of forming an electromagnetic sensing coil in a medical instrument. The method may include forming a core of a conductive material and forming a coil about the core. The core is covered with a first layer of a material and a second layer of a material may also cover the core, and at least part of the first layer. The coil may be substantially electrically isolated from the core.

According to various embodiments a surgical navigation system for a substantially minimally invasive dynamic reference frame is disclosed. The dynamic reference frame may include a body portion selectively attachable to a portion of the anatomy. It may also include a navigation portion to at least one of sense and transmit a characteristic. A holding section is able to hold the body portion relative to the portion of the anatomy. The holding section may substantially non-invasively hold the body portion relative to the portion of the anatomy.

According to various embodiments a surgical navigation system for navigating a procedure relative to a patient having an electrical isolating portion. The navigation system may include an electrical source and an instrument including a conducting element disposable near the patient. A transmission medium may interconnect the electrical source and the instrument. An electrical isolator may electrically isolate the instrument from the electrical source.

According to various embodiments, a navigation system for determining the location of a member relative to an anatomy may include a tracking system and a sensor to be sensed by the tracking system. An anti-rotation mechanism may be provided to interconnect the sensor with the anatomy. The anti-rotation mechanism contacts at least two points on the anatomy to resist rotation of the sensor relative to the anatomy.

According to various embodiments a navigation system for determining a position of a sensor relative to a portion of an anatomy including soft tissue may include a localizer operable to produce a field relative to the anatomy and a tracking sensor for sensing the field produced relative to the tracking sensor to determine a position of the tracking sensor in the field. A housing may include and/or house the sensor. The housing is operable to allow movement of the sensor relative to the soft tissue when affixed to the anatomy subcutaneously.

According to various embodiments a method of navigating a procedure relative to an anatomy with a tracking system including a localizer and a tracking sensor positioned relative to the anatomy includes providing a plurality of coils in the tracking sensor in a fixed geometry. The tracking sensor may be positioned at a location relative to the anatomy and the position of each of the plurality of coils may be determined. At least one of the plurality of the coils positioned may be determined based at least in part on the determined sensed position of the plurality of coils. Wherein determining the position includes determining a geometry of each of the coils and comparing the determined geometry to the fixed geometry.

According to various embodiments a method of navigating a procedure relative to an anatomy with a tracking system including a localizer and a tracking sensor positioned relative to the anatomy is disclosed. The method may

include providing a plurality of coils in the tracking sensor and positioning the tracking sensor at a location relative to the anatomy. A position of each of the plurality of coils may be determined and averaging each of the determined position of the plurality of coils. The position of the tracking sensor may be determined based at least in part on the averaging of each of the determined positions.

According to various embodiments a method of navigating a procedure relative to an anatomy with a tracking system including a localizer and a tracking sensor positioned relative to the anatomy may include providing a plurality of coils in the tracking sensor and positioning the tracking sensor at a location relative to the anatomy. Data regarding the position of the plurality of coils may be collected with a weight datum for each of the plurality of coils. A weight for the data collected regarding each of the plurality of coils may be determined along with a position of each of the plurality of coils.

According to various embodiments a method of using a tracking system to assist in reduction of interference in relation to the tracking system may include forming a field with a mobile localizer. An interference member may be determined and the mobile localizer may be moved to reduce the effect of the interference member.

According to various embodiments a method of navigating an anatomical position of an anatomy with an ultrasound system may include positioning the ultra-sound system relative to a selected portion of the anatomy and determining a plurality of points relative to a first portion of the anatomy subcutaneously. A first point may be selected within the determined plurality of points relative to the first portion of the anatomy. Also, a plurality of points may be determined relative to a second portion of the anatomy subcutaneously and a second point may be selected within the determined plurality of points relative to the second portion of the anatomy. A relationship between the first point and the second point may be determined.

According to various embodiments a system for navigating a tool may include a tracking system. A tracking sensor operable to be tracked by the tracking system may also be provided. An engagement member may interconnect the tracking sensor with a tool. The tracking system may be operable to track the tool.

Further areas of applicability will become apparent from the detailed description provided hereinafter. It should be understood that the detailed description and various examples, while indicating various embodiments, are intended for purposes of illustration only and are not intended to limit the scope of the description or the appended claims.

BRIEF DESCRIPTION OF THE DRAWINGS

The present teachings will become more fully understood from the detailed description and the accompanying drawings, wherein:

FIG. 1 is a diagram of a navigation system according to various embodiments of the present teachings;

FIGS. 2A and 2B are diagrams representing undistorted and distorted views from a fluoroscopic C-arm imaging device;

FIG. 3 is a top perspective view of a non-invasive dynamic reference frame according to various embodiments;

FIG. 4 is a cross-sectional view of the non-invasive dynamic reference frame of FIG. 3;

5

FIG. 5 is an environmental application of the non-invasive dynamic reference frame of FIG. 3;

FIG. 6 is a sensor bobbin that may be used in the non-invasive dynamic reference frame of FIG. 3;

FIG. 7 is an environmental view of another non-invasive dynamic reference frame according to various embodiments;

FIG. 8 is an environmental view of another non-invasive dynamic reference frame according to various embodiments

FIG. 9 is an exploded perspective view of another non-invasive dynamic reference frame according to various embodiments;

FIG. 10A is a side elevational view of a stylet;

FIG. 10B is a detail interior view of a connection portion of the stylet of FIG. 10A;

FIG. 11 is a cross-sectional view of a probe including a navigation sensor;

FIG. 12 is an enlarged view of the probe about circle 12 in FIG. 11;

FIG. 13 is a cross-sectional view of a suction instrument according to various embodiments;

FIG. 14 is an enlarged view about the circle 14 of FIG. 13;

FIG. 15 is a view of a tip of the stylet of FIG. 9A;

FIG. 16 is a cross-sectional view of the stylet tip of FIG. 15 from circle 16;

FIG. 17 is a method of forming an electromagnetic sensor according to various embodiments;

FIG. 18 is a schematic view of an isolator circuit according to various embodiments;

FIG. 19 is a detailed partial cross-sectional view of a portion of the patient including a recessed DRF;

FIG. 20 is a perspective view of a DRF including an anti-rotational mechanism according to various embodiments;

FIG. 21 is an exploded perspective view of a DRF including an anti-rotational mechanism according to various embodiments;

FIG. 21A is an elevational environmental detail view of the DRF of FIG. 21;

FIG. 22 is an exploded perspective view of a DRF including an anti-rotation mechanism according to various embodiments;

FIG. 23 is a perspective view of a DRF including an anti-rotation mechanism according to various embodiments;

FIG. 24 is a DRF including an anti-rotation mechanism according to various embodiments;

FIG. 25A is a perspective view of an instrument including a tracking sensor according to various embodiments;

FIG. 25B is a perspective view of an instrument including a tracking sensor according to various embodiments;

FIG. 26 is an environmental view of the instrument including a tracking sensor of FIG. 25A in use;

FIG. 27A is a perspective view of a DRF according to various embodiments;

FIG. 27B is a perspective view of a DRF according to various embodiments;

FIG. 28A-C is an exemplary use of a DRF according to various embodiments;

FIG. 28D is a detail environmental view of a use of the DRF of FIG. 27;

FIG. 29 is a detail perspective view of a mobile localizer;

FIG. 30 is an environmental view of the mobile localizer of FIG. 29 in use;

FIGS. 31-33 are flow charts illustrating methods of determining a position of a sensor according to various embodiments,

6

FIG. 34A is a detail partial cross-sectional view of a portion of anatomy including a scanning element;

FIG. 34B is a detail from circle in FIG. 34A;

FIG. 35 is an environmental view of implants with tracking sensors according to various embodiments;

FIG. 36 is a plan view of an instrument with a tracking sensors according to various embodiments;

FIG. 37 is a detail plan view of an instrument including a tracking sensor on a stylet according to various embodiments;

FIG. 38 is a plan view of an instrument including a tracking sensor on a stylet according to various embodiments;

FIG. 39 is an exploded view of a guide with a tracking sensor according to various embodiments;

FIG. 40 is a detail cross-sectional view of the guide of FIG. 39 according to various embodiments;

FIG. 41 is an exploded view of a tracking sensor assembly according to various embodiments;

FIG. 42 is an exploded view of a tracking sensor assembly according to various embodiments;

FIG. 43 is an exploded view of a tracking sensor assembly according to various embodiments;

FIG. 44 is a plan view of a dynamic reference frame according to various embodiments;

FIG. 45A is a cross-sectional view taken along line 45 of FIG. 44;

FIG. 45B is a cross-sectional view taken along line 45 of FIG. 44 including a protective element according to various embodiments;

FIG. 46 is a bottom plan view of the DRF illustrated in FIG. 44;

FIG. 47 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 48 is a detailed environmental view of a DRF being positioned relative to a patient according to various embodiments;

FIG. 49 is a side plan view of a DRF according to various embodiments;

FIG. 50 is a cross-sectional view of a DRF taken along line 50-50 of FIG. 49;

FIG. 51 is a bottom plan view of a DRF according to various embodiments;

FIG. 52 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 53 is a detailed environmental view of a DRF according to various embodiments being positioned relative to a patient;

FIG. 54 is a side plan view of a DRF according to various embodiments;

FIG. 55 is a cross-sectional view of a DRF, according to various embodiments, taken along line 55-55 of FIG. 54;

FIG. 56 is a bottom plan view of a DRF according to various embodiments;

FIG. 57 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 58 is a partial detail environmental view of a DRF being positioned relative to a patient;

FIG. 59 is a side plan view of a DRF according to various embodiments;

FIG. 60 is a cross-sectional view of a DRF, according to various embodiments, taken along line 60-60;

FIG. 61 is a bottom plan view of a DRF according to various embodiments;

FIG. 62 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 63 is an assembly view of a DRF and a tool according to various embodiments;

FIG. 64 is a side plan view of a DRF according to various embodiments;

FIG. 65A is a cross-sectional view taken along line 65-65 of FIG. 64;

FIG. 65B is a cross-sectional view taken along line 65-65 of FIG. 64 including a protective element, according to various embodiments;

FIG. 66 is a bottom plan view of a DRF according to various embodiments;

FIG. 67 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 68 is an assembled view of a DRF and a tool according to various embodiments;

FIG. 69 is a side plan view of a DRF according to various embodiments;

FIG. 70 is a across-sectional view of a DRF taken along line 70-70 of FIG. 69;

FIG. 71 is a bottom plan view of a DRF according to various embodiments;

FIG. 72 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 73 is an assembled view of a DRF and a tool according to various embodiments;

FIG. 74 is a side plan view of a DRF according to various embodiments;

FIG. 75A is a cross-sectional view taken along line 75-75 of FIG. 74;

FIG. 75B is a cross-sectional view taken along line 75-75 of FIG. 74 including a protective element according to various embodiments;

FIG. 75C is a cross-sectional view taken along line 75-75 of FIG. 74 including a protective element according to various embodiments;

FIG. 76 is a bottom plan view of a DRF according to various embodiments;

FIG. 77 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 78 is an assembled view of a DRF and a tool according to various embodiments;

FIG. 79 is a side plan view of a DRF according to various embodiments;

FIG. 80 is a cross-sectional view taken along line 80-80 of FIG. 79;

FIG. 81 is a bottom plan view of a DRF according to various embodiments;

FIG. 82 is a top perspective exploded view of a DRF according to various embodiments;

FIG. 83 is an assembled view of a DRF and a tool according to various embodiments;

FIG. 84 is an environmental view of a tracking sensor assembly, according to various embodiments, positioned in a patient;

FIG. 85 is a plan view of an instrument with a selected tracking device;

FIGS. 86A and 86B illustrate a representation of navigation vectors;

FIG. 87A is a perspective view of an instrument with a selected tracking device;

FIG. 87B is a cross-section view of an instrument with a selected tracking device;

FIG. 88 is a plan view of an instrument with a selected tracking device;

FIGS. 89A and 89B illustrate a representation of navigation vectors;

FIG. 90 is a plan view of an instrument with a selected tracking device;

FIG. 91A is a plan detail view of an instrument with a selected tracking device;

FIG. 91B is a display device view of an instrument and image data;

FIG. 92 is an environmental/display device view of an instrument with a selected tracking device; and

FIGS. 93A and 93B are schematic views of an instrument with a selected tracking device.

DETAILED DESCRIPTION OF VARIOUS EMBODIMENTS

The following description of various embodiments is merely exemplary in nature and is in no way intended to limit the teachings, its application, or uses. As indicated above, the present teachings are directed towards providing improved, non-line-of-site image-guided navigation of an instrument, such as a stylet, probe, suction tube, catheter, balloon catheter, implant, lead, stent, needle, guide wire, insert and/or capsule, that may be used for physiological monitoring, delivering a medical therapy, or guiding the delivery of a medical device, orthopedic implant, or soft tissue implant in an internal body space to any region of the body.

FIG. 1 is a diagram illustrating an overview of an image-guided navigation system 10 for use in non-line-of-site navigating of an instrument. It should further be noted that the navigation system 10 may be used to navigate any type of instrument, implant or delivery system, including guide wires, needles, drug delivery systems, cell delivery systems, gene delivery systems, biopsy systems, arthroscopic systems, etc. Moreover, these instruments may be used to navigate or map any regions of the body.

The navigation system 10 may include an optional imaging device 12 that is used to acquire pre-, intra-, or post-operative or real-time images of a patient 14. The optional imaging device 12 is, for example, a fluoroscopic x-ray imaging device that may include a C-arm 16 having an x-ray source 18, an x-ray receiving section 20, an optional calibration and tracking target 22 and optional radiation sensors 24. The calibration and tracking target 22 includes calibration markers 26 (see FIGS. 2A-2B), further discussed herein. A C-arm, or optional imaging device controller 28 captures the x-ray images received at the receiving section 20 and stores the images for later use. The C-arm controller 28 may also be separate from the C-arm 16 and/or control the rotation of the C-arm 16. For example, the C-arm 16 may move in the direction of arrow 30 or rotates about a longitudinal axis 14a of the patient 14, allowing anterior or lateral views of the patient 14 to be imaged. Each of these movements involve rotation about a mechanical axis 32 of the C-arm 16. In this example, the longitudinal axis 14a of the patient 14 is substantially in line with the mechanical axis 32 of the C-arm 16. This enables the C-arm 16 to be rotated relative to the patient 14, allowing images of the patient 14 to be taken from multiple directions or about multiple planes. An example of a fluoroscopic C-arm x-ray that may be used as the optional imaging device 12 is the "Series 9600 Mobile Digital Imaging System," from OEC Medical Systems, Inc., of Salt Lake City, Utah. Other exemplary fluoroscopes include bi-plane fluoroscopic systems, ceiling fluoroscopic systems, cath-lab fluoroscopic systems, fixed C-arm fluoroscopic systems, isocentric C-arm fluoroscopic systems, 3D fluoroscopic systems, etc.

In operation, the imaging device **12** generates x-rays from the x-ray source **18** that propagate through the patient **14** and calibration and/or tracking target **22**, into the x-ray receiving section **20**. The receiving section **20** generates an image representing the intensities of the received x-rays. Typically, the receiving section **20** includes an image intensifier that first converts the x-rays to visible light and a charge coupled device (CCD) video camera that converts the visible light into digital images. Receiving section **20** may also be a digital device that converts x-rays directly to digital images, thus potentially avoiding distortion introduced by first converting to visible light. With this type of digital C-arm, which is generally a flat panel device, the optional calibration and/or tracking target **22** and the calibration process discussed below may be eliminated. Also, the calibration process may be eliminated or not used at all for cardiac therapies. Alternatively, the imaging device **12** may only take a single image with the calibration and tracking target **22** in place. Thereafter, the calibration and tracking target **22** may be removed from the line-of-sight of the imaging device **12**.

Two dimensional fluoroscopic images that may be taken by the optional imaging device **12** are captured and stored in the C-arm controller **28**. Multiple two-dimensional images taken by the imaging device **12** may also be captured and assembled to provide a larger view or image of a whole region of a patient, as opposed to being directed to only a portion of a region of the patient. For example, multiple image data of a patient's leg may be appended together to provide a full view or complete set of image data of the leg that can be later used to follow contrast agent, such as Bolus tracking.

These images are then forwarded from the C-arm controller **28** to a navigation computer controller or work station **34** having a display **36** and a user interface **38**. It will also be understood that the images are not necessarily first retained in the controller **28**, but may also be directly transmitted to the navigation computer **34**. The work station **34** provides facilities for displaying on the display **36**, saving, digitally manipulating, or printing a hard copy of the received images. The user interface **38**, which may be a keyboard, mouse, touch pen, touch screen or other suitable device, allows a physician or user to provide inputs to control the imaging device **12**, via the C-arm controller **28**, or adjust the display settings of the display **36**. The work station **34** may also direct the C-arm controller **28** to adjust the rotational axis **32** of the C-arm **16** to obtain various two-dimensional images along different planes in order to generate representative two-dimensional and three-dimensional images.

When the x-ray source **18** generates the x-rays that propagate to the x-ray receiving section **20**, the radiation sensors **24** sense the presence of radiation, which is forwarded to the C-arm controller **28**, to identify whether or not the imaging device **12** is actively imaging. This information is also transmitted to a coil array controller **48**, further discussed herein. Alternatively, a person or physician may manually indicate when the imaging device **12** is actively imaging or this function can be built into the x-ray source **18**, x-ray receiving section **20**, or the control computer **28**.

The optional imaging device **12**, such as the fluoroscopic C-arm **16**, that do not include a digital receiving section **20** generally require the optional calibration and/or tracking target **22**. This is because the raw images generated by the receiving section **20** tend to suffer from undesirable distortion caused by a number of factors, including inherent image distortion in the image intensifier and external electromag-

netic fields. An empty undistorted or ideal image and an empty distorted image are shown in FIGS. **2A** and **2B**, respectively. The checkerboard shape, shown in FIG. **2A**, represents the ideal image **40** of the checkerboard arranged calibration markers **26**. The image taken by the receiving section **20**, however, can suffer from distortion, as illustrated by the distorted calibration marker image **42**, shown in FIG. **2B**.

Intrinsic calibration, which is the process of correcting image distortion in a received image and establishing the projective transformation for that image, involves placing the calibration markers **26** in the path of the x-ray, where the calibration markers **26** are opaque or semi-opaque to the x-rays. The calibration markers **26** are rigidly arranged in pre-determined patterns in one or more planes in the path of the x-rays and are visible in the recorded images. Because the true relative position of the calibration markers **26** in the recorded images are known, the C-arm controller **28** or the work station or computer **34** is able to calculate an amount of distortion at each pixel in the image (where a pixel is a single point in the image). Accordingly, the computer or work station **34** can digitally compensate for the distortion in the image and generate a distortion-free or at least a distortion improved image **40** (see FIG. **2A**). A more detailed explanation of exemplary methods for performing intrinsic calibration are described in the references: B. Schuele, et al., "Correction of Image Intensifier Distortion for Three-Dimensional Reconstruction," presented at SPIE Medical Imaging, San Diego, Calif., 1995; G. Champelboux, et al., "Accurate Calibration of Cameras and Range Imaging Sensors: the NPBS Method," Proceedings of the IEEE International Conference on Robotics and Automation, Nice, France, May, 1992; and U.S. Pat. No. 6,118,845, entitled "System And Methods For The Reduction And Elimination Of Image Artifacts In The Calibration Of X-Ray Imagers," issued Sep. 12, 2000, the contents of which are each hereby incorporated by reference.

While the optional imaging device **12** is shown in FIG. **1**, any other alternative 2D, 3D or 4D imaging modality may also be used. For example, any 2D, 3D or 4D imaging device, such as isocentric fluoroscopy, bi-plane fluoroscopy, ultrasound, computed tomography (CT), multi-slice computed tomography (MSCT), magnetic resonance imaging (MRI), high frequency ultrasound (HIFU), positron emission tomography (PET), optical coherence tomography (OCT), intra-vascular ultrasound (IVUS), ultrasound, intra-operative CT or MRI may also be used to acquire 2D, 3D or 4D pre- or post-operative and/or real-time images or image data of the patient **14**. The images may also be obtained and displayed in two, three or four dimensions. In more advanced forms, four-dimensional surface rendering regions of the body may also be achieved by incorporating patient data or other data from an atlas or anatomical model map or from pre-operative image data captured by MRI, CT, or echocardiography modalities. A more detailed discussion on optical coherence tomography (OCT), is set forth in U.S. Pat. No. 5,740,808, issued Apr. 21, 1998, entitled "Systems And Methods For Guiding Diagnostic Or Therapeutic Devices In Interior Tissue Regions" which is hereby incorporated by reference.

Image datasets from hybrid modalities, such as positron emission tomography (PET) combined with CT, or single photon emission computer tomography (SPECT) combined with CT, could also provide functional image data superimposed onto anatomical data to be used to confidently reach target sights within the patient **14**. It should further be noted that the optional imaging device **12**, as shown in FIG. **1**,

11

provides a virtual bi-plane image using a single-head C-arm fluoroscope as the optional imaging device **12** by simply rotating the C-arm **16** about at least two planes, which could be orthogonal planes to generate two-dimensional images that can be converted to three-dimensional volumetric images. By acquiring images in more than one plane, an icon representing the location of a catheter, stylet, suction-probe, or other instrument, introduced and advanced in the patient **14**, may be superimposed in more than one view on display **36** allowing simulated bi-plane or even multi-plane views, including two and three-dimensional views.

These types of imaging modalities may provide certain distinct benefits for their use. For example, magnetic resonance imaging (MRI) is generally performed pre-operatively using a non-ionizing field. This type of imaging provides very good tissue visualization in three-dimensional form and also provides anatomy and functional information from the imaging. MRI imaging data is generally registered and compensated for motion correction using dynamic reference frames (DRF) discussed further herein.

Positron emission tomography (PET) imaging is generally a pre-operative imaging procedure that exposes the patient to some level of radiation to provide a 3D image. PET imaging provides functional information and also generally requires registration and motion correction using dynamic reference frames.

Computed tomography (CT) imaging is also generally a pre-operative technique that exposes the patient to a limited level of radiation. CT imaging, however, is a very fast imaging procedure. A multi-slice CT system provides 3D images having good resolution and anatomy information. Again, CT imaging is generally registered and needs to account for motion correction, via dynamic reference frames.

Fluoroscopy imaging is generally an intra-operative imaging procedure that exposes the patient to certain amounts of radiation to provide either two-dimensional or rotational three-dimensional images. Fluoroscopic images generally provide good resolution and anatomy information. Fluoroscopic images can be either manually or automatically registered and also need to account for motion correction using dynamic reference frames.

Ultrasound imaging is also generally intra-operative procedure using a non-ionizing field to provide either 2D, 3D, or 4D imaging, including anatomy and blood flow information. Ultrasound imaging provides automatic registration and does not need to account for any motion correction.

With continuing reference to FIG. 1, the navigation system **10** further includes an electromagnetic navigation or tracking system **44** that includes a localizer, such as a transmitter coil array **46**, the coil array controller **48**, a navigation probe interface **50**, an electromagnetic instrument, such as a stylet or catheter **52** and a dynamic reference frame **54**. It will be understood that the localizer may be any appropriate localizer, such as an optical, an acoustic, or other localizer depending upon the system for which the localizer is chosen. Further included in the navigation system **10** is an isolator circuit or box **55**. The isolator circuit or box **55** may be included in a transmission line or interrupt a line carrying a signal or a voltage to the navigation probe interface **50**. Alternatively, the isolator circuit included in the isolator box **55** may be included in the navigation probe interface **50**, the instrument **52**, the dynamic reference frame **54**, the transmission lines coupling the devices, or any other appropriate location. As discussed herein, the isolator box **55** is operable to isolate any of the instruments or patient coincidence

12

instruments or portions that are in contact with the patient should an undesirable electrical surge or voltage take place, further discussed herein.

It should further be noted that the entire tracking system **44** or parts of the tracking system **44** may be incorporated into the imaging device **12**, including the work station **34** and radiation sensors **24**. Incorporating the tracking system **44** may provide an integrated imaging and tracking system. Any combination of these components may also be incorporated into the imaging system **12**, which again can include a fluoroscopic C-arm imaging device or any other appropriate imaging device.

The transmitter coil array **46** is shown attached to the receiving section **20** of the C-arm **16**. It should be noted, however, that the transmitter coil array **46** may also be positioned at any other location as well. For example, the transmitter coil array **46** may be positioned at the x-ray source **18**, within or atop the OR table **56** positioned below the patient **14**, on siderails associated with the table **56**, or positioned on the patient **14** in proximity to the region being navigated, such as on the patient's chest. The transmitter coil array **46** may also be positioned in the items being navigated, further discussed herein. The transmitter coil array **46** includes a plurality of coils that are each operable to generate distinct electromagnetic fields into the navigation region of the patient **14**, which is sometimes referred to as patient space. Representative electromagnetic systems are set forth in U.S. Pat. No. 5,913,820, entitled "Position Location System," issued Jun. 22, 1999 and U.S. Pat. No. 5,592,939, entitled "Method and System for Navigating a Catheter Probe," issued Jan. 14, 1997, each of which are hereby incorporated by reference.

The transmitter coil array **46** is controlled or driven by the coil array controller **48**. The coil array controller **48** drives each coil in the transmitter coil array **46** in a time division multiplex or a frequency division multiplex manner. In this regard, each coil may be driven separately at a distinct time or all of the coils may be driven simultaneously with each being driven by a different frequency. Upon driving the coils in the transmitter coil array **46** with the coil array controller **48**, electromagnetic fields are generated within the patient **14** in the area where the medical procedure is being performed, which is again sometimes referred to as patient space. The electromagnetic fields generated in the patient space induce currents in sensors **58** positioned in the instrument **52**, such as the catheter, further discussed herein. These induced signals from the instrument **52** are delivered to the navigation probe interface **50** through the isolation circuit **55** and subsequently forwarded to the coil array controller **48**. The navigation probe interface **50** may provide all the necessary electrical isolation for the navigation system **10**. Alternatively, the electrical isolation may also be provided in the isolator box **55**. Nevertheless, as mentioned here, the isolator assembly **55** may be included in the navigation probe interface **50** or may be integrated into the instrument **52**, and any other appropriate location. The navigation probe interface **50** also includes amplifiers, filters and buffers required to directly interface with the sensors **58** in the instrument **52**. Alternatively, the instrument **52** may employ a wireless communications channel as opposed to being coupled directly to the navigation probe interface **50**.

The instrument **52**, as will be described in detail below, is equipped with at least one, and generally multiple, localization sensors **58**. The instrument **52** can be a steerable catheter that includes a handle at a proximal end and the multiple location sensors **58** fixed to the catheter body and spaced axially from one another along the distal segment of

the catheter **52**. The catheter **52**, as shown in FIG. **1** includes four localization sensors **58**. The localization sensors **58** are generally formed as electromagnetic receiver coils, such that the electromagnetic field generated by the transmitter coil array **46** induces current in the electromagnetic receiver coils or sensors **58**. The catheter **52** may also be equipped with one or more sensors, which are operable to sense various physiological signals. For example, the catheter **52** may be provided with electrodes for sensing myopotentials or action potentials. An absolute pressure sensor may also be included, as well as other electrode sensors. The catheter **52** may also be provided with an open lumen, further discussed herein, to allow the delivery of a medical device or pharmaceutical/cell/gene agents. For example, the catheter **52** may be used as a guide catheter for deploying a medical lead, such as a cardiac lead for use in cardiac pacing and/or defibrillation or tissue ablation. The open lumen may alternatively be used to locally deliver pharmaceutical agents, cell, or genetic therapies.

In an alternate embodiment, the electromagnetic sources or generators may be located within the instrument **52** and one or more receiver coils may be provided externally to the patient **14** forming a receiver coil array similar to the transmitter coil array **46**. In this regard, the sensor coils **58** would generate electromagnetic fields, which would be received by the receiving coils in the receiving coil array similar to the transmitter coil array **46**. Other types of localization sensors or systems may also be used, which may include an emitter, which emits energy, such as light, sound, or electromagnetic radiation, and a receiver that detects the energy at a position away from the emitter. This change in energy, from the emitter to the receiver, is used to determine the location of the receiver relative to the emitter. Other types of tracking systems include optical, acoustic, electrical field, RF and accelerometers. Accelerometers enable both dynamic sensing due to motion and static sensing due to gravity. An additional representative alternative localization and tracking system is set forth in U.S. Pat. No. 5,983,126, entitled "Catheter Location System and Method," issued Nov. 9, 1999, which is hereby incorporated by reference. Alternatively, the localization system may be a hybrid system that includes components from various systems.

The dynamic reference frame **54** of the electromagnetic tracking system **44** is also coupled to the navigation probe interface **50** to forward the information to the coil array controller **48**. The dynamic reference frame **54**, briefly and discussed in detail according to various embodiments herein, is a small magnetic field detector that is designed to be fixed to the patient **14** adjacent to the region being navigated so that any movement of the patient **14** is detected as relative motion between the transmitter coil array **46** and the dynamic reference frame **54**. This relative motion is forwarded to the coil array controller **48**, which updates registration correlation and maintains accurate navigation, further discussed herein. The dynamic reference frame **54** can be configured as a pair of orthogonally oriented coils, each having the same center or may be configured in any other non-coaxial or co-axial coil configuration. The dynamic reference frame **54** may be affixed externally to the patient **14**, adjacent to the region of navigation, such as on the patient's chest, as shown in FIG. **1**. The dynamic reference frame **54** can be affixed to the patient's skin, by way of a selected adhesive patch and/or a tensioning system. The dynamic reference frame **54** may also be removably attachable to fiducial markers **60** also positioned on the patient's body and further discussed herein.

Alternatively, the dynamic reference frame **54** may be internally attached, for example, to the wall of the patient's heart or other soft tissue using a temporary lead that is attached directly to the heart. This provides increased accuracy since this lead may track the regional motion of the heart. Gating may also increase the navigational accuracy of the system **10**. Gating procedures may be particularly important when performing procedures relative to portions of the anatomy that move on a regular basis, such as the heart or the lungs or diaphragm. Although, it is not necessary to provide gating, it may be selected to do so during various procedures. Various gating procedures and techniques are described, such as U.S. patent application Ser. No. 10/619,216 entitled "Navigation 'System For Cardiac Therapies'" filed on Jul. 14, 2003, and incorporated herein by reference. Dynamic reference frame **54** according to various embodiments and a fiducial marker **60**, are set forth in U.S. Pat. No. 6,381,485, entitled "Registration of Human Anatomy Integrated for Electromagnetic Localization," issued Apr. 30, 2002, which is hereby incorporated by reference.

It should further be noted that multiple dynamic reference frames **54** may also be employed. For example, an external dynamic reference frame **54** may be attached to the chest of the patient **14**, as well as to the back of the patient **14**. Since certain regions of the body may move more than others due to motions of the heart or the respiratory system, each dynamic reference frame **54** may be appropriately weighted to increase accuracy even further. In this regard, the dynamic reference frame **54** attached to the back may be weighted higher than the dynamic reference frame **54** attached to the chest, since the dynamic reference frame **54** attached to the back is relatively static in motion.

The navigation system **10** may optionally further include a gating device **62** such as an ECG or electrocardiogram, which is attached to the patient **14**, via skin electrodes **64**, and in communication with the coil array controller **48**. Respiration and cardiac motion can cause movement of cardiac structures relative to the instrument **52**, even when the instrument **52** has not been moved. Therefore, localization data may be acquired on a time-gated basis triggered by a physiological signal. For example, the ECG or EGM signal may be acquired from the skin electrodes **64** or from a sensing electrode included on the instrument **52** or from a separate reference probe. A characteristic of this signal, such as an R-wave peak or P-wave peak associated with ventricular or atrial depolarization, respectively, may be used as a triggering event for the coil array controller **48** to drive the coils in the transmitter coil array **46**. This triggering event may also be used to gate or trigger image acquisition during the imaging phase with the imaging device **12**. By time-gating or event gating at a point in a cycle the image data and/or the navigation data, the icon of the location of the catheter **52** relative to the heart at the same point in the cardiac cycle may be displayed on the display **36**, such as disclosed in U.S. patent application Ser. No. 10/619,216, entitled "Navigation System For Cardiac Therapies" filed on Jul. 14, 2003.

Additionally or alternatively, a sensor regarding respiration may be used to trigger data collection at the same point in the respiration cycle. Additional external sensors can also be coupled to the navigation system **10**. These could include a capnographic sensor that monitors exhaled CO₂ concentration. From this, the end expiration point can be easily determined. The respiration, both ventilated and spontaneous causes an undesirable elevation or reduction (respectively) in the baseline pressure signal. By measuring systolic and diastolic pressures at the end expiration point, the

coupling of respiration noise is minimized. As an alternative to the CO₂ sensor, an airway pressure sensor can be used to determine end expiration.

Briefly, the navigation system **10** operates as follows. The navigation system **10** creates a translation map between all points in the radiological image generated from the imaging device **12** and the corresponding points in the patient's anatomy in patient space. After this map is established, whenever a tracked instrument, such as the catheter **52** or a pointing device **66** is used, the work station **34** in combination with the coil array controller **48** and the C-arm controller **28** uses the translation map to identify the corresponding point on the pre-acquired image or atlas model, which is displayed on display **36**. This identification is known as navigation or localization. An icon representing the localized point or instruments are shown on the display **36** within several two-dimensional image planes, as well as on three and four dimensional images and models.

To enable navigation, the navigation system **10** must be able to detect both the position of the patient's anatomy and the position of the catheter **52** or other surgical instrument. Knowing the location of these two items allows the navigation system **10** to compute and display the position of the catheter **52** in relation to the patient **14**. The tracking system **44** is employed to track the catheter **52** and the anatomy simultaneously.

The tracking system **44** essentially works by positioning the transmitter coil array **46** adjacent to the patient space to generate a low-energy magnetic field generally referred to as a navigation field. Because every point in the navigation field or patient space is associated with a unique field strength, the electromagnetic tracking system **44** can determine the position of the catheter **52** by measuring the field strength at the sensor **58** location. The dynamic reference frame **54** is fixed to the patient **14** to identify the location of the patient in the navigation field. The electromagnetic tracking system **44** continuously recomputes the relative position of the dynamic reference frame **54** and the catheter **52** during localization and relates this spatial information to patient registration data to enable image guidance of the catheter **52** within the patient **14**.

Patient registration is the process of determining how to correlate the position of the instrument or catheter **52** on the patient **14** to the position on the diagnostic or pre-acquired images. To register the patient **14**, the physician or user may use point registration by selecting and storing particular points from the pre-acquired images and then touching the corresponding points on the patient's anatomy with the pointer probe **66**. The navigation system **10** analyzes the relationship between the two sets of points that are selected and computes a match, which correlates every point in the image data with its corresponding point on the patient's anatomy or the patient space. The points that are selected to perform registration are the fiducial markers or landmarks **60**, such as anatomical landmarks. Again, the landmarks or fiducial points **60** are identifiable on the images and identifiable and accessible on the patient **14**. The landmarks **60** can be artificial landmarks **60** that are positioned on the patient **14** or anatomical landmarks that can be easily identified in the image data. The artificial landmarks, such as the fiducial markers **60**, can also form part of the dynamic reference frame **54**.

The system **10** may also perform registration using anatomic surface information or path information as is known in the art. The system **10** may also perform 2D to 3D registration by utilizing the acquired 2D images to register 3D volume images by use of contour algorithms, point

algorithms or density comparison algorithms, as is known in the art. An exemplary 2D to 3D registration procedure, as set forth in U.S. Ser. No. 60/465,615, entitled "Method and Apparatus for Performing 2D to 3D Registration" filed on Apr. 25, 2003, which is hereby incorporated by reference. The registration process may also be synched to an anatomical function, for example, by the use of the ECG device **62**.

In order to maintain registration accuracy, the navigation system **10** continuously tracks the position of the patient **14** during registration and navigation. This is because the patient **14**, dynamic reference frame **54**, and transmitter coil array **46** may all move during the procedure, even when this movement is not desired. Therefore, if the navigation system **10** did not track the position of the patient **14** or area of the anatomy, any patient movement after image acquisition would result in inaccurate navigation within that image. The dynamic reference frame **54** allows the electromagnetic tracking device **44** to register and track the anatomy. Because the dynamic reference frame **54** is rigidly fixed to the patient **14**, any movement of the anatomy or the transmitter coil array **46** is detected as the relative motion between the transmitter coil array **46** and the dynamic reference frame **54**. This relative motion is communicated to the coil array controller **48**, via the navigation probe interface **50**, which updates the registration correlation to thereby maintain accurate navigation.

The navigation system **10** can be used according to any appropriate method or system. For example, pre-acquired images or atlas or 3D models may be registered relative to the patient and patient space. Various registration regimens and techniques include those described in U.S. patent application Ser. No. 10/619,216 entitled "Navigation System For Cardiac Therapies" filed on Jul. 14, 2003. Generally, the registration system allows the images on the display **36** to be registered and accurately display the real time location of the various instruments, such as the instrument **52**, and other appropriate items, such as the pointer **66**. In addition, the pointer **66** may be used to register the patient space to the pre-acquired images or the atlas or 3D models. In addition, the dynamic reference frame **54** may be used to ensure that any planned or unplanned movement of the patient or the receiver array **46** is determined and used to correct the image on the display **36**.

As discussed above, the dynamic reference frame **54** may include any appropriate dynamic reference frame, such as the selectively fixable dynamic reference frame **70** illustrated in FIG. 3. The dynamic reference frame **70** generally includes a superior side **72** and an inferior side **74**.

With continuing reference to FIG. 3 and additional reference to FIG. 4, the dynamic reference frame **70** includes a recess **76** as a portion of the inferior side **74**. The recess **76** may be provided for any appropriate purpose, such as receiving a selective adhesive. In addition, as discussed herein, the recess may be used to allow the gathering of soft tissue relative to the dynamic reference frame **70**. As described, the dynamic reference frame **70** may be affixed to the patient **14** in any appropriate position.

An adhesive positioned in the adhesive recess **76** generally allows the dynamic reference frame **70** to be fixed to the selected point on the patient **14**. As discussed further herein, a tensioning apparatus may also be provided on the dynamic reference frame **70** to further assist holding the dynamic reference frame in a selected position. Further, the dynamic reference frame **70** defines a bore **78** to removably receive a selected sensor or coil. As described herein, the sensor may be fitted into the sensor bore **78** and removed from the sensor

bore 78 as selected. For example, should the dynamic reference frame 70 also be used as a fiducial marker 60 it may be radio- or image-opaque, and the sensor bobbin 90 may be removed from the bore 78 during imaging of the patient 14, such as acquiring MRI images. This eliminates any distortion that may be caused by the bobbin 90. Nevertheless, the sensor bobbin 90 may also be permanently provided within the sensor bore 78 for ease of use of the apparatus. It may be desirable to provide the dynamic reference frame 70 as a substantially disposable exterior portion and the sensor may be reusable. In either case, the dynamic reference frame 70 may be formed of a plastic or other non-conductive material.

If the dynamic reference frame 70 is used as a fiducial marker, the dynamic reference frame 70 may define a localization divot 80. The divot or recess 80 allows the pointer 66 or any appropriate mechanism to determine the location of the dynamic reference frame 70 relative to the patient 14 or the patient space. Generally, the pointer 66 is able to engage the divot 80 in a selected manner in patient space, such that the navigation system 44 is able to determine the position of the dynamic reference frame 70 relative to the patient 14. The pointer 66 is also engaged or used to point out the divot 80 in the pre-acquired image to register the image space with the patient space. Therefore, detected movement of the dynamic reference frame 70 may be used to determine movement of the patient 14. It will be understood that the divot 80 may be positioned in any appropriate portion of the dynamic reference frame 70 but is generally provided in an easily accessible and viewable area. Moreover, there may be multiple divots 80 or landmarks, as discussed herein. The multiple divots 80 may be used as fiducial markers. There dynamic reference frame 70 may also include a radio-opaque material to be imaged in various imaging techniques.

With further reference to FIG. 3, the dynamic reference frame 70 may include a concave recess 82 defined as a portion of the superior part 72 of the dynamic reference frame 70. The recess 82 may be provided for any appropriate purpose such as engaging a tensioning member 84. The tensioning member 84 may include an adhesive strip that is applied relative to the dynamic reference frame 70 to ensure a substantial selected fixation of the dynamic reference frame 70 relative to the patient 14.

With reference to FIG. 5, an exemplary use of the dynamic reference frame 70 is illustrated. The dynamic reference frame 70 is affixed to the patient 14 using an adhesive that is included in the adhesive recess 76. In addition, the tensioning strip 84 is placed atop the recess 82 to further hold the dynamic reference frame 70. The tensioning strip 84 helps by tensioning the dermis 86 of the patient 84 relative to the dynamic reference frame 70. Generally, the dermis 86 will form pucker or tension lines 88 to illustrate or ensure that the dynamic reference frame 70 is substantially fixed to the patient 14. In this way, the soft tissue to which the dynamic reference frame 70 is fixed and is not able to move relative to the dynamic reference frame 70, thereby providing a relatively stable and secure attachment to the patient 14.

Although it is illustrated that the dynamic reference frame 70 may be tensioned relative to the skin of the pectoral region of the patient the dynamic reference frame 70 may be tensioned relative to any appropriate portion of the anatomy. For example, the dynamic reference frame 70 may be fixed relative to a posterior portion of the patient 14 relative to the spine, if a spinal procedure is occurring. In addition, the dynamic reference frame 70 may be tensioned to the dermis

on the forehead of the patient, if a procedure relative to the cranium is being performed. Nevertheless, the dynamic reference frame 70 may be fixed to the dermis with substantial force using the tensioning device 84.

Although the tensioning device 84 is illustrated to be a separate strip of material having an adhesive, it will be understood that the tensioning device 84 may be integrated into the dynamic reference frame 70. For example, a tensioning system may be fixed to the superior portion 72 of the dynamic reference frame 70 and a backing released to expose an adhesive region to allow the tensioning system to tension the dermis relative to the dynamic reference frame 70. In addition, tensioning strips, that form the tensioning device 84 may be affixed to or formed integrally with any appropriate portion of the dynamic reference frame 70 to allow for easy use during an operative procedure. For example, tape or a belt may be used that may be separate or integral with the dynamic reference frame 70. Therefore, it will be understood that the tensioning device 84 need not be limited according to any selected embodiments and is provided to allow for tensioning the dermis relative to the dynamic reference frame 70.

As is generally known by one skilled in the art, the dermis of an individual is generally not substantially taught over the sub-dermal anatomy. That is, a portion of the anatomy may move relative to the dermis without the dermis moving. Although this may be desired for general anatomical or natural movements, it may be desired to know the precise movements of any portions of the anatomy of the patient 14 during an operative procedure where the navigation system 44 is being used.

The instrument 52, such as the catheter, may be engaged to a subdermal region of the patient 14. Movement of any subdermal portion may be selected to be known during the operative procedure. In addition, the position of the instrument 52 relative to the subdermal anatomical portions may be selected to be substantially known. Therefore, the dynamic reference frame 70 may be fixed to the patient 14 to allow for ensuring that the image on the display 36 substantially correctly illustrates the position of the anatomy of the patient 14. If subdermal portions are allowed to move without the dynamic reference frame 70 moving, however, it may be possible that the display 36 may not correctly display the proper location of the instrument 52 relative to the subdermal anatomy of the patient 14. Therefore, the tensioning strip 84 may allow for more closely tracking the movement of subdermal portions or portions of the anatomy of the patient 14 without using more invasive techniques.

Generally, the dynamic reference frame 70 may be affixed to the dermis or external portions of the patient 14. This allows the dynamic reference frame 70 to be fixed to the patient and used to reference the position of the patient 14 relative to the position of the other elements, such as the instrument 52 and the pointer 66, and to also ensure the appropriate registration of the images on the display 36 in a substantially non-invasive manner. Simply the dynamic reference frame 70 need not penetrate the dermis to be fixed to a rigid portion of the anatomy, such as a bone portion. Therefore, the dynamic reference frame 70 can be easily fixed and removed from the patient 14 as selected.

An electromagnetic bobbin or multiple coil member 90 may be positioned in the recess 78 of the dynamic reference frame 70. The sensor bobbin 90 includes a body 92 that is generally formed from material that is not conductive to allow the coils to operate and sense a position in a field. In addition, the body 92 may be manipulated by a handle or manipulable portion 94 extending from the body 92. In

addition, the handle **94** may allow leads or contacts from an external source, such as illustrated in FIG. 1, to be interconnected to the body portion **92** into the coils **96** and **98**.

The first coil **96** and the second coil **98** are generally positioned at angles relative to one another. These angles may be any appropriate angle such as a generally orthogonal angle or other appropriate angle. The two coils **96**, **98** being positioned at angles relative to one another, allow for six degrees of freedom sensing including translation, angle, pitch, yaw, and rotation. Therefore, the position or movement of the dynamic reference frame **70** can be determined by sensing the electromagnetic field of the coil array **46** with the first coil **96** and the second coil **98**.

Generally, the body **92** of the bobbin **90** and the exterior or the bodies of the dynamic reference frame **70** are formed of an appropriate material. For example, the material may be a non-metallic and non-conducting material such as an appropriate ceramic, plastic, and the like. The material may be selected from a material that will not interfere with either transmitting or receiving information regarding the magnetic field and not interfere with imaging of the patient **14**. Therefore, the material is a substantially non-conducting material, but may also be visible in the image data.

In addition, the dynamic reference frame **70** may be used to address what may be referred to as skin shift. As described above the skin may move relative to the subdermal anatomic portions. Therefore, the dynamic reference frame **70** may be fixed to the patient **14** in a manner to substantially eliminate error that may be introduced by a skin shift. In addition to the tensioning device **84**, the tensioning device may be any appropriate portion. For example, the tensioning device **84** may be a band which substantially extends around the selected anatomical portion of the patient. For example, the dynamic reference frame **70** may be fixed to a band that substantially extends around the chest of a patient during a selected procedure. In addition, the dynamic reference frame **70** may be included on or integral with a band that substantially extends around the cranium, the arm, the thigh, or any other appropriate member. In addition, the band may be substantially elastic to engage the selected anatomical portion. The elastic band may be provided to substantially tension the tissue relative to the dynamic reference frame, but not simply in a localized tensioning manner. The dynamic reference frame **70** can, therefore, be fixed to any appropriate portion of the body either with the localized tensioning member **84** or a non-localized tensioning member. The band may form a general tensioning while a tape portion may form a more localized tensioning. The tensioning members allow for tensioning the dermal tissue over the subdermal anatomy to substantially eliminate skin movement relative to the subdermal area.

In addition, the dynamic reference frame **54** may be substantially non-invasively placed near a substantially rigid portion of the anatomy. For example, the dynamic reference frame may include a rhinal dynamic reference frame **100**, as illustrated in FIG. 7. The rhinal dynamic reference frame **100** may include a body **102** and an optional tensioning device **104**. The rhinal dynamic reference frame **100** is formed to generally fit over a bridge **106** of a nose **108** of the patient **14**. Generally, the bridge **106** of the nose **108** is covered with a substantially thin layer of dermal tissue. Therefore, the bridge of the nose **106** is substantially rigid relative to the patient **14**. In addition, the tensioning member **104** may be provided to stabilize any portion of the skin that may move relative to the bridge **106** of the nose **108**. However, the adhesive portion fixed on the bottom of the dynamic reference frame **100** may simply be the only

adhesive necessary to fix the rhinal dynamic reference frame **100** to the bridge **106** of the nose. Nevertheless, the rhinal dynamic reference frame **100** may allow for the dynamic reference **100** to be fixed to the patient **14** in a substantially rigid and repeatable place.

Not only may the rhinal dynamic reference frame **100** be fixed to the bridge **106** of the nose, but the dynamic reference **100** may be substantially molded to a particular portion of the nose **108**. Therefore, a molded or moldable inferior portion **110** of the rhinal dynamic reference frame **100** may be fitted to a selected portion of the nose **108**. The dynamic reference frame **100** may be positioned and repositioned relative to the bridge **106** of the nose **108** a plurality of times with substantially repeatable placements of the dynamic reference frame **100**.

The repeatable substantially precise placement enables the dynamic reference frame **100** to be removed and replaced onto the bridge **106** of the nose **108** without substantially introducing error into the positioning of the dynamic reference frame **100**. This allows initial pre-operative images to be taken with the dynamic reference frame **100** in place and used as a fiducial marker. The rhinal dynamic reference frame **100** may then be removed from the patient **14** prior to the operative procedure. Subsequently, during the operative procedure, the rhinal dynamic reference frame **100** may be repositioned on the patient **14**. Because the molded portion **110** of the rhinal dynamic reference frame **100** is substantially fitted to a particular portion of the bridge **106** of the nose **108**, the rhinal dynamic reference frame **100** can be substantially positioned in the same position as during the pre-operative images. Therefore, the rhinal dynamic reference frame **100** allows for substantially error free referencing of the patient and registration of the patient **14** to the pre-operative images that may be displayed on the display **36**. This allows the rhinal dynamic reference frame **100** to be used as both the dynamic reference frame **54** and as a fiducial marker for registering of the pre-operative images.

In addition, it will be understood that the dynamic reference frame **100** may be positioned in any appropriate manner. As illustrated above, the dynamic reference frame **70** may be fixed to a substantially flat portion of the anatomy of the patient **14**. Alternatively, the anatomic or rhinal dynamic reference frame **100** may be molded to a substantially uniquely shaped portion of the anatomy of the patient **14**. It will be understood that other portions of the anatomy may also be substantially molded to fit a particular portion of the anatomy.

With reference to FIG. 8, a further alternative embodiment of the dynamic reference frame includes an anatomic or inner-cochlear dynamic reference frame **111**. The inner cochlear dynamic reference frame **111** is generally molded to fit a portion or the cochlear portion of the ear **112**. The cochlear portion of the ear **112** generally includes a substantially unique topography that may be used to fit the dynamic reference frame **111** in substantially only one position. Therefore, as discussed in relationship to the rhinal dynamic reference frame **100** that includes the moldable portion, the inner-cochlear dynamic reference frame **111** may also be formed, at least partially, of a moldable material.

For example, a distal portion **111a** of the inter cochlear implant **111** may be formed of a substantially moldable material that may be press fit into the cochlear portion **112** of the ear of the patient **14**. After being molded to the cochlear portion **112** of the ear of the patient **14**, the moldable material may be cured to substantially maintain

the molded shape. An exterior or proximal portion **111B** of the inner-cochlear implant **111**, may be formed of a moldable or a non-moldable material. Therefore, the inner-cochlear implant **111** may be formed of two materials. Nevertheless the proximal portion **111b**, or any appropriate portion, may also include a first sensing coil **113** and a second sensing coil **114**. The sensing coils **113**, **114** may be positioned in any appropriate manner but may be positioned at angles relative to one another. Therefore, the inner-cochlear implant may provide six degrees of freedom information regarding motion of the inner-cochlear dynamic reference frame **111** during use.

The position of the sensors **113**, **114** may be referenced and calibrated after molding of the inner-cochlear implant **111**. Therefore, the position of the head of the patient **14** may be known based upon the sensed position of the inner-cochlear dynamic reference frame **111**. In addition, as discussed in relation to the other dynamic reference frames, the coils **113**, **114** may be passive or active. If the coils **113**, **114** are active, the inner-cochlear dynamic reference frame **111** may include a power source, such as battery.

The inner-cochlear dynamic reference frame **111** may also be substantially molded as a separate procedure. For example, such as forming an inner-cochlear hearing aid, the inner-cochlear dynamic reference **111** may be molded to the cochlear portion of the ear of the patient **14** and the inner-cochlear dynamic reference frame **111** may be formed separately after the impression is made. Nevertheless, the molding of the inner-cochlear dynamic reference frame **111** relative to the cochlear portion of the ear **112** with the patient **14**, allows for a substantially repeatable placement of the inner-cochlear dynamic reference frame **111** relative to the patient **14**. Therefore, images displayed on the display **36** may be substantially easily registered relative to the known location and repeatable location of the inner-cochlear dynamic reference frame **111**.

It will be understood that the molded portions may be substantially permanently molded or reusably molded. For example, a curable material may be included, in any appropriate dynamic reference frame, such as the inner-cochlear dynamic reference frame **111**. The moldable portion of the cochlear implant **111** may be molded to a portion of the ear or press fit into the ear and then cured to substantially maintain the molded shape. Therefore, the dynamic reference frames may be substantially non-invasively positioned relative to the patient to allow for dynamic referencing of the patient **14** during the operative procedure.

In addition, the dynamic reference frame may be formed almost entirely of the substantially molded material. Therefore, the dynamic reference frame may include a molding material that may be molded to a selected portion of the anatomy and then cured to maintain the shape of the anatomy and also may be formed to include an area to receive the sensor bobbin **90**. Although it will be understood that any appropriate coils may be used to form the sensor and may include substantially separate coils that can be positioned into the moldable material substantially separately and removably.

It will also be understood that the dynamic reference frame **54** may be fixed to any appropriate portion of the anatomy. As discussed above, the dynamic reference frame may be positioned relative to the nose **108**, the chest of the patient **14**, the head of the patient **14**, also the dynamic reference frame may be formed as a bite block that may be fitted onto selected portions of the oral anatomy. Also, the dynamic reference frame may be fitted onto or in a tooth cap

that may be fit over a tooth, an oral bite block that may be held within the teeth or jaws of the patient or any other appropriate location.

The dynamic reference frame **54** may either be substantially wireless and powered by an internal power source or may be wired. For example, a hard wire dynamic reference frame **120** is illustrated in FIG. 9. The hard wire dynamic reference frame **120** includes a bottom body portion **122** and a top body portion or cap **124**. The cap **124** is generally able to mate with the bottom portion **122** in an appropriate manner and may include a recess **126** to receive the head of a screw to lock the top **124** to the bottom **122**. Formed in the bottom portion **122** is a groove **128** that is able to receive a wire such as twisted pair wire **130**. The wire **130** may include leads that are soldered to a printed circuit board (PCB) **132**. The PCB **132** may include traces that are translated or connected to intermediate wires **134** and **136** that are able to transfer power or a signal to and/or from a first coil **138** and a second coil **140**. The coils **138**, **140** are generally coils of wire that generate an induced current by an electric field or may transmit an electric field.

The line **130** may operatively interconnect the hard wired dynamic reference frame **120** to the navigation interface **50**. Therefore, the hard wire dynamic reference frame **120** may transmit the navigation signals received by the coils through the transmission line **130**. Alternatively, as discussed above, an internal power source may be provided such that the information received by the coils **138**, **140** may be wirelessly transmitted to the navigation controller **34** using known wireless technology.

The hardwire dynamic reference frame **120** may include any appropriate dimensions. For example the hardwire dynamic reference frame **120** may be about 2 mm to about 10 millimeters in height. Generally, the less the height of the dynamic reference frame the less the possibility for error in transmitting the location of the coils relative to the patient **14**. Also, the inferior surface at the base **124** may include a radius to mate with a selected anatomical region, such as a forehead.

The hard wire dynamic reference frame **120** may still be fixed to the dermis of a patient **14** in any appropriate manner. For example, the tensioning member **84** may be provided over the top of the top portion **124** of the hard wire dynamic reference frame **120**. In addition, an adhesive may be provided on the inferior portion of the hard wire dynamic reference frame **120**.

In addition, the hard wire dynamic reference frame **120**, particularly the upper portion **124** and the lower body portion **122**, may be formed of an appropriate material. For example, materials may include non-conductive materials such as ceramic or various polymers. In addition, the hard wire dynamic reference frame may be formed of non-conductive carbon fiber materials. In addition, the coils **138**, **140** may include conductive carbon fiber materials as the coil component. In addition, the PCB **132** need not be present and the wires may simply be fixed to the coils **138**, **140** from the lead **130**. Nevertheless, various selections may be chosen to include the PCB **132** or to wire the lead **130** directly to the coils **130**, **140**.

Therefore, it will be understood that the dynamic reference frame may be formed in any appropriate shape. In addition, the dynamic reference frame **54** may be substantially moldable or non-moldable depending upon the selected shape or position for positioning the dynamic reference frame. Nevertheless, the dynamic reference frame **54** is substantially positioned non-invasively on the patient **14**. Therefore, rather than fixing the dynamic reference

frame in an invasive manner, such as with bone screws or the like, the dynamic reference frame may be fixed to the patient in a substantially error reducing manner using the tensioning members or a substantially molded portion.

In addition, more than one dynamic reference frame may be provided on the patient **14**. More than one dynamic reference frame may be provided for error correction or error detection. Nevertheless, the inclusion of the non-invasive dynamic reference frames may be allowed for substantially simple positioning of the dynamic reference frames during an operative procedure. In addition, the dynamic reference frames **54** may be easily positioned relative to the patient **14** in a substantially quick manner as well. Therefore, the unexpected need for a dynamic reference frame **54** may be solved by simply fixing the dynamic reference frame **54** to the patient **14** using the various constructs. The dynamic reference frame **54** may also be fixed to the patient **14** in any appropriate manner. Such adhesives may be painted on, sprayed on, or include “double-sided” tape. Regardless, the adhesive allows for simple placement of the dynamic reference frame **54** for a selected procedure.

The size, such as the height, the width, etc. of the dynamic reference frame may be selected depending upon selected characteristics. For example, the hard wire dynamic reference frame **120**, which may also be substantially wireless dynamic reference frame, may include a select height that is substantially shallow or low to allow for a reduced possibility of movement of the dynamic reference frame **120**. In addition, the height or distance of the coils **138**, **140** from the anatomy of the patient **14** is small. Therefore, any movement of the hard wire dynamic reference frame **120** is substantially closer to movement of the patient **14** than if the coils were positioned further from the patient **14**. Therefore, the size of the dynamic reference frame may also be chosen depending upon the selective amount or error of the system.

In addition, as briefly mentioned above, the coils **138**, **140** may be provided in the hard wire dynamic reference **120** or in any appropriate dynamic reference frame. Generally, the coils **138**, **140** are substantially similar in functioning to the coils **96** and **98** on the sensor bobbin **90**. Simply, the coils are positioned in a slightly different position, but angled relative to one another to provide sensing of six degrees of freedom. Therefore, whether the coils are substantially positioned on the single member, such as in the sensor bobbin **90**, or separated such as the coils **138**, **140** in the hard wire dynamic reference **120**, still provide the required information for sensing the location of the dynamic reference frame.

Any of the dynamic reference frames (which also may be wireless) may be used as the dynamic reference frame **54**, such as the dynamic reference frame **70**, the intercochealor dynamic reference frame **111**, or the hardwire dynamic reference frame **120** may include various selected characteristics. For example, the sensor portion, such as the included respective coils, may be removable for various reasons. If an imaging technique, such as an MRI is used to image the patient and the dynamic reference frame is left as a fiducial marker, the electromagnetic coils may be removed. Therefore, it will be understood that the coils may either be permanently included within the dynamic reference frame or may be removable therefrom, particularly when the dynamic reference frame is used as a fiducial marker.

In addition, the dynamic reference frame may be used as a fiducial marker. For example, the dynamic reference frame may include a region that is substantially matable or molded to mate with a portion of the anatomy in substantially one way. In addition the dynamic reference frame may also include a portion that is inherently contoured to mate with a

portion of the anatomy without including a moldable portion. This allows substantially precise replacement and repeatability of placement of the dynamic reference frame to be achieved.

Because of the precise repeatable placement of the dynamic reference frame it may also serve as a fiducial marker that may be used in preoperative imaging to be a fiducial marker for use during registration intra-operatively. Therefore, the dynamic reference frames may include materials that are substantially radio-opaque or opaque to the imaging process. Various materials may be used to form the radio-opaque dynamic reference frames, such as selected metals, selected compounds, and various mixtures.

Moreover, if the dynamic reference frame is used as a fiducial marker, it may be selected to include portions on the dynamic reference frame that may be viewed on the pre-acquired image and during the procedure. For example, as discussed in relationship to the dynamic reference frame **70**, the dynamic reference frame may include the reference dimple or landmark **80**. It will be understood that a plurality of the reference dimples may be provided on the dynamic reference frame **70** for use during an operative procedure to reference the patient space to the image space. The number of reference points, which either may be physical portions, such as the dimples, or markings on the dynamic reference frame, are generally viewable and identifiable on the pre-acquired images, so that each may be matched to a selected portion of the dynamic reference frame during the operative procedure. This allows for multiple degrees of freedom and allows an appropriate and precise registration of the patient space to the image space.

In addition, it will be understood that each of the dynamic reference frames include a portion that allow the dynamic reference frame to be held relative to the patient **14**. Therefore, each of the dynamic reference frames includes a selected holding portion. For example, the holding portion may include the adhesive that adheres the dynamic reference frame to a selected portion of the patient **14**. In addition, the moldable portion, such as the moldable portion of the intercochealor implant **111a**, may be a holding portion and no other portion may be provided to hold the intercochealor dynamic reference frame **111** relative to the patient **14**. Regardless, each of the dynamic reference frames may include a holding portion that allows the dynamic reference frame to be held relative to a patient. It may be that the holding portion defines a substantially matable and repeatable placement of the dynamic reference frame relative to the patient **14**, such that the dynamic reference frame may also be repeatedly precisely placed and may be used for various purposes, such as a fiducial marker.

Various instruments may be included for use in a selected procedure, such as a stylet **150**, with reference to FIGS. **10A** and **10B**. The stylet **150** generally includes a connection wire or cable **152** and an electronic lead and/or handle **154**. Extending from the handle **154** is a stylet portion **156** that is generally moved within the cavity of the patient **14**. For example, the stylet **150** may be the instrument **52** rather than the catheter. Therefore, the stylet **150** is an exemplary instrument **52**.

Generally, the stylet portion **156** includes a distal or tip end **158** and a proximal end **160**. The stylet may be positioned through a cannula and may be used to guide the cannula, though the stylet **150** may be used for any appropriate reason. Positioned near the distal end **158** is a sensor **162**. The sensor **162** may be a coil, or multiple coils, to interact with the field transmitted by the transmitter coil array **48**. Briefly and described in detail herein, the sensor

162 is generally wrapped around an internal highly electro-magnet permeable core insulated with a heat shrink or any appropriate dielectric material. The details of the process and the sensors 162 are described in further detail herein.

With additional reference to FIGS. 10A and 10B, the handle 154 of the stylet 150 may include an area to connect the wires from the coils. A first set of contacts 241 provide an area for contact to each of the leads of the first coil 240. A second pair of contacts 245 is provided for the leads of the second coil 244. In this way, power or sensor leads may be attached to the handle or sensor region 154 for receiving the sensitive information of the sensors or coils 240, 244.

With reference to FIG. 11, a probe 166 is illustrated, as a further alternative for the instrument 52, and generally includes a handle portion 168 and a probe tip 170. The handle 168 is generally formed of a non-metallic material that can be easily grasped and isolated from the electrical lead 172. The electrical lead generally provides a current to a portion of the tip 170.

With continuing reference to FIG. 11 and additional reference to FIG. 12, a tip sensor 174 may be positioned in the tip 170 of the probe 166. The tip 170 generally is formed of a non-metallic and/or a non-conductive material. Inside of the tip 170 is a metal shaft 176 that can be formed of an appropriate electromagnetic permeable material. Formed around the metal shaft 176 is a sensor coil 178. A second sensor coil 180 may also be provided. The first and second sensor coils 178, 180 are generally co-axial and formed along the axis of the permeable rod 176. The tip 170 and the rod 176 with the coils 178, 180 are generally positioned within a tube portion 182 of the probe 166. As discussed, the lead 172 provides power to the sensor portion including the coils 178, 180. The sensor portion including the coils 178, 180 may be similar to the sensor portion 162 of the stylet 150 and described in detail herein. Regardless, the sensor portion is generally positioned substantially at the tip or the distal end of the probe 166 to allow for substantially accurate measurement of the position of the tip of the probe.

With reference to FIGS. 13 and 14, a suction device 190 is illustrated. Again, the suction device 190 generally includes a handle 192 which includes a connection area 194 to be connected to a suction source. A cannula opening 196 runs the length of the suction portion such that material may be suctioned through a distal tip 198 of the suction instrument 190. Also provided through the handle 192 may be a power source that is able to energize a sensor or sense an electromagnetic field that is acting upon a sensor 200 positioned in the tip 198.

With particular reference to FIG. 14, the suction instrument 190 near the tip 198 generally includes an internal ductile and possibly conductive or nonconductive tube 202. Positioned over the tube is an inner dielectric layer 204. Coils 206 and 208 may also be positioned over the dielectric layer 204. Finally, the sensor 200 may be sealed with an outer dielectric layer 210. Again, the formation of the sensor 200 is described herein including the two coils, 206, 208. Generally, the coils are positioned near the tip 198 of the suction instrument 190 and to provide for substantially accurate position data for the tip 198 of the suction instrument 190. Therefore, the tip 198 of the suction instrument 190 may be moved and the sensor 200 is positioned substantially near the tip 198 so that intended or unintended motion of the tip 198 relative to the handle may be determined.

The sensors, according to any embodiment described above, are generally positioned near a distal end or movable end of an instrument, such as the suction instrument 190, the

probe 166, or the stylet 150. Generally, the position of the various instruments, particularly the ends of the instruments, is determined by the known location of a sensor or a transmitting coil and the known size, length, and other physical attribute of the instrument. Therefore, the sensor may be positioned away from or disposed a distance from the extreme end of the instrument. Although a very small and tolerable error may be introduced when the instruments are flexed or move unexpectedly, but this may also cause the exact location of the tip to not be known. This may require many repositioning and attempts to complete a procedure. This error may be detected or substantially eliminated when the sensor is positioned near the distal tip of the instrument, particularly when the instrument is flexible. Therefore, rather than determining or knowing the various physical characteristics of the instrument, the actual sensed portion is the end that may move expectedly or unexpectedly. Therefore, providing the sensor near the distal tip may provide for substantial accurate position data of the instrument.

Generally, the position of the instrument is displayed on the display 36 and is not generally viewable by a user because it is within the cavity of the patient 14. Therefore, the user is generally dependent upon the accuracy of the display 36 to ensure the proper location, orientation and other attributes of the instrument relative to the patient 14. For example, as illustrated in FIG. 1, the instrument 52, such as the catheter, is positioned relative to a specific portion of a heart of the patient 14. Similarly, the stylet 150 may be positioned relative to an extremely particular and precise portion of the brain. Therefore, it may be selected or desirable to substantially eliminate any error when determining the position of the instrument relative to the patient 14.

Although the following description relates generally to the formation of the sensor 162 for the stylet 150, it will be understood that the sensor may be used in any appropriate instrument 52, such as the catheter, the probe 166, the suction instrument 190 or any other appropriate instrument. In addition, the instruments may include any selected tip shape or sizes depending upon a selected use of the instrument. For example, an arthroscope or camera may be provided in the tip for viewing on the display 36 or any other appropriate display. Nevertheless, the sensor may be positioned near the lens portion such that the exact and precise location of the lenses is known.

In addition, various portions of the instrument may be ductile or movable such that the tip is not at a fixed location relative to other portions of the instrument. Therefore, the tip may be movable while the handle is substantially fixed at a known location. Therefore, the sensor positioned at the tip is able to provide the position of the tip even though the handle has not moved.

It will also be understood that various handle calibration and verification points may be included as well as areas for directing wiring within the various instruments and through the handle. It will be understood that these various portions are provided for directing wiring, allowing verification and calibration and are not described in unneeded detail. In addition, the instruments may be substantially disposable or reusable, depending upon the various material specifics being used and the sterilization techniques.

According to various embodiments, a method of forming the sensors that can be positioned near the tip in a substantially small volume or space, such as in the stylet tip 158, is described. With reference to FIG. 9 and FIG. 14, the stylet tip 158 is illustrated in detail in FIG. 14. With reference to FIG. 15, a detail of a first sensor coil 240 and an extreme

distal tip portion **158A** is illustrated. The various coatings or layers around a central rod **242** is illustrated and described herein. Generally, the central rod **242** is a conductive rod and may include various materials such as “302 spring” stainless steel. The material for the rod **242** that is also generally the flexible or steerable portion of the stylet **150** may be any appropriate material. Generally, the material for the rod **242**, however, is highly permeable to electromagnetic fields. This generally increases the signal to noise ratio or the gain of the signal of the sent field to a selected amount. Generally, the signal to noise ratio may be increased at least about 5% depending upon the various materials chosen to form the selected construct.

With reference to FIGS. **15** and **16** the stylet tip **158** generally includes a first coil and may also include a second coil **244**. The first and second coils **240**, **244**, or any appropriate number of coils may be provided on the tip **158**. In addition, the coils **240**, **244** may be substantially co-axial or formed at an angle relative to one another. That is, the wire or material used to form the coils **240** and **244** may be wrapped at an angle relative to each other around the rod **242**. When the coils are not wrapped at an angle relative to one another, a degree of freedom may not be detected, such as rotation. For various instruments however, such as the uniform stylet tip **158**, rotational information may not be necessary and selectively not determined. Nevertheless, for other instruments, such as a suction tube, an ablation tube, or a lens, it may be desired to produce the coils at an angle relative to one another such that rotational direction and location may be determined.

As described in detail in flow chart in FIG. **17**, prior to forming a coil, a first dielectric barrier or layer **246** may be provided over the rod **242**. The first dielectric barrier layer **246** generally is not placed over the extreme end of the tip **158a** and generally includes a back set or offset distance of about 0.025 mm to about 1.5 mm depending upon the size of the rod **242**. For example, the offset distance *C* may be a selected multiple of a diameter of the rod **242**. Not to be limited by the theory, but including the back-set may reduce the possibility of damage to the first dielectric layer **246** during use of the stylet **150**. Generally, the extreme tip **159a** may be used to touch hard surfaces and this may damage the dielectric material. Nevertheless, it will be understood that the first layer of the dielectric material **246** may extend over the extreme tip of the tip **158**.

The coils **240**, **244** may then wrapped around the first dielectric layer **246**. After the coils are positioned over the first dielectric layer **246**, a second dielectric layer **248** is provided over the coils **240**, **244**. Again, the second dielectric layer **248** may be offset a distance *D* from the extreme end of the tip **158a**. Nevertheless, it will also be understood that the second dielectric layer **248** may also extend to the end of the tip **158a**.

It will be understood that the first layer **246** and the second layer **248** need not necessarily be a dielectric material. This is merely exemplary and not intended to limit the scope thereof. For example the material may simply be used to isolate the windings from an exterior environment and the first layer omitted entirely. Alternatively, the wire that forms the coils **240**, **244** may be separately or individually coated prior to forming the coils **240**, **244**. Therefore, the isolation may be achieved without forming a separate layer or coating, such as the first and second layers **246**, **248**.

Although the apparatus and a very brief process for forming the apparatus is described above, the following description, in addition to the flowchart illustrated in FIG. **17**, describes a detailed method of forming the stylet tip

including the sensor **162** according to various embodiments. A method of forming a sensor, such as electromagnetic sensor that may be either passive or active, is described in relationship to the flowchart and a method **260**. Generally, the method begins a start block **262**.

After the process is started in block **262**, a material may be selected for form a core in block **264**, such as the core **242**. As described above, the selected core material in block **264** may be a highly electromagnetic permeable material. Although it is not necessary that the core be highly permeable to electromagnetic fields or be conductive, it may be desirable to provide a highly permeable core for various applications. For example, when forming the stylet tip **158**, it may be selected to provide the stylet tip to have diameter no greater than about 1.25 mm. In addition, it may be selected to include a stylet diameter of less than about 1 mm. It may also be desirable to provide a stylet tip **158** in any appropriate diameter or selected property. Therefore, the stylet **158** may be deflectable or bendable according to selected characteristics. Also, at the small diameter the highly permeable material may increase the gain of the field sensed by the coils. Therefore the location information may be more easily determined and sensed.

After the selected core material is chosen in block **264**, the core is formed in block **266**. The core may be formed according to any selected specifications, such as those described above. Therefore, the core formed in block **266** may include a length, a cross-section, and other various properties that may be selected for the stylet tip **158**. Although the material may be selected for the core in block **264** and the core formed in block **266**, it will be understood that these steps are optional as steps for forming the selected sensor. The method **260** is exemplary for forming the stylet tip **158**. Although the process **260** is exemplary for forming the stylet tip **158**, it will be understood that various portions thereof may be used in any process for forming a sensor according to the below described process and a tip sensor in a substantial small area. Therefore, steps that are substantially optional are positioned in blocks that are outlined with dashed or phantom lines and will be indicated as optional herein. Therefore, it will be understood that various steps, although described, are not required to form the sensor as described herein. Therefore, the process is merely exemplary and various specific details are provided only for clarity and not intended to limit the description or the appended claims.

After the core is optionally formed in block **266**, a first layer of material is positioned over the core in block **268**. The first layer of material positioned in block **268** may be a dielectric. Though the material for the first layer may be any appropriate material and is merely exemplary a dielectric. The first layer of the dielectric material may be positioned over the core in any appropriate manner. For example, the first layer of the dielectric material may be positioned over the core as a heat shrink or shrink wrap process. This being that a portion of the material may be formed as tube and slide over the core and then shrunk to substantially engage the core along its length. Alternatively, the material may be painted on or sprayed on the core formed in block **266**.

For any or all of these processes, a plurality of layers of the material may be positioned on the core to form the first dielectric layer of a selected thickness. The thickness of the dielectric layer may be any appropriate thickness according to selected characteristics. For example, the thickness of the first layer of the dielectric material may be about 0.00025 inches to about 0.03 inches (about 0.00635 mm to about

0.762 mm). Generally, however, the first layer of the dielectric material may be about 0.001 inches (about 0.0254 mm) in thickness.

The dielectric material may also be any appropriate dielectric material to achieve selected results. For example, it may be selected to have dielectric breakdown strength of about at least about 4,000 volts per about 0.001 inches (mil) (about 0.0254 mm) in thickness. Although any appropriate dielectric break down strength may be selected. Also, it may be selected to choose other properties for the first dielectric layer placed in block 268. Various materials may be used such as polyester shrink tubing or ULTRATHIN WALL POLYESTER (PET) shrink tubing provided by Advanced Polymers Inc. of Salem, N.H. Although any appropriate material may be used, it may be selected to include the dielectric breakdown strength of at least about 1000 volts per mil.

After the first layer of dielectric material is positioned on the core, the layer may be inspected in block 270. The inspection may be any appropriate inspection such as a visual inspection, magnification inspection, or various electrical tests to ensure that the selected installation is achieved. Also, the first layer of dielectric material may be inspected to ensure that it has been positioned on the core in a selected manner. As described above, it may be selected to only cover a selected portion of the core and not extend the first layer of dielectric material substantially to the tip of the core. As illustrated in FIG. 15, it may be selected to position the first layer of dielectric material 246, the distance C from the extreme end 158a of the tip 158.

After the optional inspection of block 270, a first sensor coil is formed in block 272. The sensor coil, such as the coil 240 illustrated in FIG. 15, may be formed using any appropriate materials. For example, a 48 gauge magnetic wire that is coated with a single built polyurethane with butyl bonds may be wrapped around the core including the first layer of dielectric material to form the first sensor coil.

The wire may be wrapped around the first layer of the dielectric material in any appropriate manner. For example, the coils may be wrapped substantially co-axially with a longitudinal axis of the core. Alternatively, the wire may be wrapped substantially at an angle to the core for selected reason, such as sensing rotation of the core during use. As an example, a first sensor coil may include a first layer of coils including approximating 300 turns and a second layer positioned over top of the first layer also having approximately 300 turns. Therefore, the first coil formed in block 272 may include approximately 600 turns. Nevertheless, it will be understood that only a single layer or any number of layers may be used and that any appropriate number of turns may be used to form the first sensor coil in block 272.

The first coil formed in block 272 is exemplary wound around the first layer positioned in block 268. It will be understood that the wire used to form the coil in block 272 may first be coated or may be a coated wire. When the wire is coated or covered positioning the first layer of material in block 268 may be omitted. The coating on the wire may provide all of the properties, such as electrical, environmental and the like, that the material in the first layer formed in block 268 may otherwise provide.

An optional second coil, which may also be formed of coated or covered wire, may be formed in block 274. Therefore, it will be understood that any appropriate number of coils may be formed for reasons discussed herein but may include a first coil formed in block 272 and a second coil formed in block 274. If there are two coils, the second coil may be positioned a selected distance from the first coil. For

example, the first coil may have an edge that is about 0.25 mm to about 10 mm from an end of the second coil. Nevertheless, it will be understood that the coils may be positioned at any appropriate position on the tip 158 and relative to one another.

After the first sensor coil is formed in block 272 and optionally the second sensor coil in block 274, the ends of the wires forming the sensor coils may optionally be twisted in block 276. The ends of the wires that form the coils formed in blocks 272 and optionally in block 274 may be twisted in any appropriate manner. For example, the wires may be twisted in about 10 to about 30 twist per inch and may be uniformly twisted rather than twisting one around the other. Although it will be understood that the wires may be formed in any appropriate manner and that twisting the wires in block 276 is merely optional.

After the wires are optionally twisted in block 276, the ends of the coils are attached to locations on the stylet handle in block 278. Generally, the leads of the coil are attached to selected positions, such as to a printed circuit board or to other wire leads, that allow for interconnection to various components, such as the navigation interface 50 (FIG. 1). The coil leads that are attached from block 278 may be attached to any appropriate portion and may be from either the first sensor coil formed in block 272 or the optional second sensor coil formed in block 278.

After the leads from the coils are attached in block 278, or at any appropriate time, a second layer of material may be positioned in block 280. The second layer of material positioned in block 280 may be any appropriate material and is only exemplary a dielectric. The second layer of dielectric material may be positioned over both of the first layer of dielectric material, that was positioned in block 268, and over the sensor coil formed in block 272, and optionally in block 274. The material that is used to form the second layer of the dielectric material may be the same or different than the material chosen to form the first layer of the dielectric material in block 268. In addition, the method of positioning the second layer of the dielectric material in block 280 may also be the same or different that the method used to position the first layer of dielectric material in block 268. For example, the first layer of the dielectric material positioned in block 268 may be a substantially heat shrink or shrink tubing that is positioned over the core formed in block 266 and then shrunk according to any selected method, such as heating. Alternatively, the second layer of dielectric material positioned in block 280 may be sprayed or painted on over. In addition, the material may be the same, such as the Ultra Thin Wall polyester (PET) heat shrink tubing produced by Advanced Polymers Incorporated or may be any other appropriate material.

Nevertheless, the second layer of the dielectric material may include the same or different dielectric break down strength in the first layer. For example, the dielectric breakdown strength of the second layer of the dielectric material may be at least 4000 volts per mil or may be any other appropriate amount.

Briefly, as an example, the first layer of the dielectric material may provide insulation between the sensor coil formed in block 272 and the core formed in block 266. Therefore, the sensor coil formed in block 272 is electrically isolated from the core formed in 266. This allows the core formed in 266 to also be a conductive material and may also act as a core and a gain amplifier for the sensor coil, as described further herein. In addition, the second layer of the dielectric material may act as an electrical insulator relative

to a patient or a portion exterior to the core and as an environmental seal to the sensors formed in block 272 and optionally in block 274.

It will also be understood that the second layer of the material positioned in block 280 may also be omitted. It may be omitted for any reason, such as the wires that form the coil formed in block 272 are previously coated. Therefore, the second layer of material formed in block 280 may be omitted. Regardless, the second layer of material may be any appropriate material and need not be a dielectric. The second layer of material in block 280 may be positioned for any appropriate reason, such as a liquid seal, an electrical isolation, etc.

After positioning the second layer of the dielectric material in block 280 the second layer of dielectric material may be optionally inspected in block 282. As in block 270, the material may be inspected according to any appropriate method, such as visual inspection, magnification inspection, and electrical testing.

After the second layer of the dielectric material is optionally inspected in block 282 the ends over the core may be sealed. As illustrated in FIG. 16, the first layer of dielectric material 246 and the second layer of dielectric material 248 may not extend over the extreme tip 158a of the core 242. Therefore, it may be selected to seal the extreme end 158a over the dielectric layers 246, 248 to achieve a substantially water tight or other material tight seal.

The seal formed optionally in block 284 may be formed in any appropriate manner. For example, the extreme tip 158a and any selected length along the tip 158 may be dipped into a selected material, such as Loctite® 4014 produced by Henkel Corporation of Rocky Hill, Conn. The material may substantially seal the interior so that no fluid can be wicked or drawn towards the coil 240 through capillary action. Therefore, the coating of the dielectric layers, blocks 268 and 280 may be sealed in any appropriate manner to ensure that no fluid is allowed to destroy or short the coils formed on the tip 158.

In addition to the steps described above, various other steps such as testing the dielectric strength in block 286, testing the connection of the coil after attaching the coil leads in 278, testing the coils in block 288, and inspecting the construct for achieving the appropriate dimensions in block 290 may be performed. Then the process ends in block 292.

Although various optional steps may have been performed in the method 260 it will be understood that the sensors generally formed by positioning on a first layer over dielectric material over a core, forming a sensor coil around the first layer of the dielectric material in block 272, and positioning a second layer of dielectric material in block 280 over the coil may be performed. In addition, the dielectric materials may be any appropriate materials and are generally provided only for safety considerations. Therefore, simply forming the coil around the core may be performed for any appropriate purpose. Providing the dielectric layers are able to protect the user and the patient from any possible surges and insure that the instrument is not corrupted by environmental degradation.

Furthermore, additional assembly steps may be performed depending upon the selected instrument. As illustrated in FIG. 10, the cable 152 may be interconnected with the connection area 154 and interconnected with the navigation probe interface 50. Alternatively, if the other instruments, such as the probe 166 or the suction tube 190 are formed, the relative handles may be provided and affixed thereto and various other connections may also be performed. Never-

theless, it will be understood that these steps are not necessary for forming the sensor near the tip of the construct.

With reference to FIG. 16 the exterior dimension or diameter E of the tip 158 and of the stylet portion 156 of the stylet 150 may be any appropriate dimension and may be about 0.09 mm to about 1.5 mm in diameter. It will be understood that the dimension may be any appropriate exterior dimension as the stylet portion 160 may be formed in any shape, but may be a cylinder. The diameter E generally includes the dimension of the core 242 the first dielectric layer 246 and the second dielectric layer 248. In addition, a diameter F that includes the diameter or size of the coil 240 may be about 0.9 mm to about 1.50 mm in diameter. Therefore, the diameter F may be greater than the diameter E depending upon whether the space between the coils is selected to be equal to the size as around the coils 240.

Regardless of the actual size, it is desired to include a diameter of the stylet portion 156 that is substantially small for use in various purposes. For example, the stylet portion 156 may generally be provided with a cannula that is positioned in various portions of the anatomy, such as the brain. Therefore, it may be desirable to provide the stylet portion 156 and a plurality of other instruments through the cannula without moving the cannula. Therefore, the stylet may be of a selected diameter that will substantially freely move within the cannula.

Although it may be selected to keep the maximum diameter F under a selected size, it will be understood that any appropriate or selected size of diameter may be used. Simply having a substantially small diameter may provide various selected properties, as having it selected for various instruments and purposes. Again, as described above, various portions of the instrument and the method may be optional and not necessary. Although the core 242 may be formed of a substantially conductive material that is surrounded by the first layer of dielectric material 246, that is able to isolate the coil 240 from the conductive material of the core 242, and the second layer of dielectric material 248 provided to enclose the coil 240 from an exterior environment; it will be understood that various other portions, such as providing the core 242 as the core 176 in the probe 166 or the metal tube 202 on the suction instrument 190 may also be provided.

The core 242 may be formed of any appropriate material, but may be formed of the permeable material that may include ferrous materials such as ferrites like those provided by Fair-Rite Products Corp. of Wallkill, N.Y. The permeable material may provide a gain to the signal of the coils, such as the first coil 240 and the second coil 244 in the stylet 150. The material may provide a gain that is relative to its permeability, especially above the permeability of air. Therefore, the gain experienced may be dependent upon the type of material chosen for the core 242, or any core about which the coils are formed in various embodiments.

In addition, it will be understood that any appropriate number of coils may be provided. For example, the stylet 150 may include the first coil 240 and the second coil 244. As described above, the windings of the coils 240, 244 may be substantially co-axial so that only five degrees of freedom are determined. Nevertheless, the windings of the coils may also be formed at an angle relative to one another so that rotational orientation of the stylet 150 may also be determined. In addition, any appropriate number of coils may be provided along the length of the instrument for various purposes.

For example, two coils that are coaxial may be provided for error detection. The first coil may be provided at a known

distance from a second coil. Therefore, the sensed position of the first coil **240** relative to the second coil **244** may be used to detect errors between the positions of the two to determine the exact location of the tip **158** of the stylet **150**. In addition, a compensation circuit may be provided to compensate for the sensed signal from the first coil **240** relative to the second coil **244**. Therefore, providing two coils in the stylet **150** may be provided for any number of reasons or for all appropriate reasons. In addition, it will be understood that the number and types of coils may be provided in each of the instruments described above and any other appropriate instrument. Nevertheless, a substantially small or narrow sensor coil may be provided according to the steps described above and may also be provided according to the various optional steps described above.

With reference to FIGS. **1** and **18** the isolator circuit **55** may be provided to isolate any portion of the instrument **52** that may engage the patient **14** from the electrical source, such as the work station **34**. As illustrated in FIG. **1**, the instrument **52**, which may include the stylet **150**, the probe **166**, the suction instrument **190**, and/or any other appropriate instrument, is inserted into the patient **14**. Each of the instruments may include the sensor **58**, as disclosed herein and above, to which an electrical current has provided. In addition, the dynamic reference frame **54**, according to any of the embodiments or various other embodiments, as described herein or understood to be included within the scope of the present disclosure, may also include an electrical lead from the navigation probe interface **50**. In addition, any other systems such as the probe **66** may each have an electrical current provided thereto. The isolator circuit **55** may be positioned anywhere to isolate any of these instruments from the electrical source.

The isolator circuit **55** may include any appropriate isolation transformer **300**. The transformer **300** may include a first coil **302** that is operable to transmit or receive a signal. The first coil **302** may generally be on an output side that receives a signal and transmits it through the navigation probe interface **50** and to the workstation **34** or the coil array controller **48**.

The first coil **302** may be separated from a plurality of second coils **304a**, **304b**, and **304c** by a dielectric or appropriate medium **306**. As described herein each of the coils **304a-304c** may be in-line with a selected instrument or device. It will be understood, however, that a single second coil may be provided with a plurality of taps connected thereto. The dielectric medium **306** eliminates a current that may attempt to transfer from the first coil **302** to the second coils **304a**, **304b**, and **304c** or vice versa. Nevertheless, an electromotive force may be provided into either of the first coil **302** or the second coils **304a**, **304b**, and **304c** that may couple across the dielectric material **306**. In this way, the second coils **304a**, **304b**, and **304c** is electrically isolated from the first coil **302**, such that only a potential is able to transfer across the dielectric medium **306**.

The second coil **304** may include leads to the dynamic reference frame **54**, the instrument **52**, such as a catheter, and the probe **66**. As discussed above the instrument **52** may also be the stylet **150**, the probe **166**, and/or the suction tube **190**, or any appropriate instrument. Both the first coil **302** and the second coils **304a**, **304b**, and **304c** may also include a ground lead. Generally, the first coil **302** is operably connected to the work station **34** through the navigation probe interface **50**. The navigation probe interface may include appropriate power sources and amplifiers as necessary. Therefore, the navigation probe interface **50** may be electrically isolated from the various portions of the assembly

10 that may engage the patient **14**. In this way, a current may not be transferred through the electrical isolator **55** to any of the instruments, sensors, or portions that touch the patient, such as the instrument **52** and the dynamic reference frame **54**.

In addition, as discussed briefly below, the first coil **302** may include a different number of windings than the second coils **304a**, **304b**, and **304c**. For example, if it is desired to include a stronger signal going back to the navigation probe interface **50**, a number of windings in the first coil **302** may be greater than the number in the second coil **304**. Therefore, the electrical isolator **55** may also act as an amplification circuit for receiving a signal from the various components, such as the dynamic reference frame **54** and the instrument **52**.

As illustrated in FIG. **1**, the isolator circuit **55** may be provided on any of the lines from the navigation probe interface **50**. Therefore, any electrical surge may be immediately stopped before engaging the patient **14** or instrument **52**. Thus, the isolator circuit **55** may be positioned on each of the lines leading to each of the instruments, the probe **66** or the dynamic reference frame **54**. Furthermore, the isolator circuit **55** may be incorporated into the navigation probe interface **50** or into any of the instruments **52**, the dynamic reference frame **54**, or the probe **66**. The isolator circuit **55** may be positioned anywhere to eliminate the current that may be unintentionally provided to the patient **14**.

For example, with reference to FIG. **9B**, the isolator circuit may be included within the circuit capsule **154** of the stylet **150**. Therefore, the power provided to the stylet **150** may be interrupted when a selected voltage or current is reached. The isolator circuit may allow stopping a voltage before it is able to pass through the circuit to reach the sensors. The isolator circuit **55** in addition to the dielectric layers positioned over the coils **240**, **244**, may assist in protecting the patient **14** from undesired electrical shock. In addition, the isolator circuit **55** may be incorporated into any other appropriate portion of the other instruments with a dynamic reference frame.

In addition to isolating the patient **14** from undesired electrical current or shock, the isolator circuit **55** may also act as an amplifier to increase the signal to noise ratio. For example, the isolator circuit **55** may be a step up transformer that is designed to increase the signal to noise ratio a selected amount. For example, a selected side, such as the signal output side, of the circuit may include a number of windings that is greater than the signal input side such that the signal is stepped up and the signal to noise ratio is increased. Therefore, the isolator circuit **55** may not only electrically isolate the patient **14** from an undesirable surge, but may also increase the signal to noise ratio to increase the efficiency of the navigation system **10**.

Therefore, the navigation system **10** may be provided to include a dynamic reference frame **54** that is substantially non-invasive such that the patient **14** does not endure further trauma than required from the operative procedure. Generally, the navigation system **10** is able to provide a less invasive or minimally invasive procedure to achieve less trauma to the patient **14**. Therefore, providing a substantially non-invasive dynamic reference frame may assist in decreasing the overall trauma or invasiveness of the procedure.

In addition, the sensor coils may further reduce the size of the instrument for various purposes. In addition, the size of the coils may allow the coils to be positioned near the distal end of the instrument to more precisely determine the position of the instrument. Therefore, the position determi-

nation of the instrument can be more accurate. For example positional accuracy can be increased by at least about 5% over placing the sensors away from the tip. The procedure may then be performed with fewer attempts thereby again further reducing the possible trauma of the procedure.

Also, the isolator circuit **55** may increase the signal to noise ratio to better determine the position of the various sensors and therefore determine the position of the instrument. In addition, the isolator circuit **55** may assist in isolating the patient **14** from any electrical sources of the navigation system **10**. Therefore, the navigation system **10** may increase the efficacy.

According to various embodiments dynamic reference frames (DRFs) may be provided. DRFs may include a tracking sensor. The tracking sensor may be tracked by a tracking system. The DRF may be used by the system to register or maintain registration of patient space to image space.

Various DRFs may be fixed or inserted in various portions of the anatomy, such as those described above and herein. Various DRFs may be fixed in bores in hard or boney portions. Various DRFs may be fixed in at least one orientation relative to selected portions of the anatomy. It will be further understood that although a DRF is discussed in particular herein, any appropriate sensor may be provided. The sensor may be a portion of a tool, a probe, or any other instrument. Also the DRF, according to various embodiments may include coils for use in an electromagnetic tracking system, but may also include or alternatively include optical sensors, acoustic sensors, or any appropriate sensor portion. The DRF may be also referred to as a DRF assembly. The sensor in the DRF may generally be referred to as a tracking sensor for use in a DRF or a DRF sensor. Thus, it will be understood, that a DRF may include a DRF sensor that includes a tracking sensor used as a DRF.

Further, as described above and herein, a plurality of the DRFs may be used to assist in maintaining registration of the patient space to the image space. As described above, the registration allows for the tracking system to track an instrument relative to the patient and ensure that the display shows an accurate position and orientation representation of the instrument relative to the patient. The DRFs, as described above, assist in maintaining the registration of the patient space to the image space during a selected procedure regardless of movement of the patient. It will be understood, however, that any appropriate number of DRFs may be provided on the patient or in a selected position for maintaining the registration of the patient space to the image space.

For example, a single DRF that provides six degrees of freedom information may be used. The single six degree of freedom DRF (6 DOF DRF) tracks six types of movements in space that may be identified with the single DRF and maintained relative to the patient. Generally, the 6 DOF DRF is substantially fixed both rotationally and translationally relative to a portion of the patient. For example, an anti-rotation DRF may be positioned relative to the patient, such as in a bony portion, that includes a selected number of tracking sensors or coils to ensure the 6 DOF DRF. In this regard, three coils, positioned for example, orthogonal to one another will provide 6 degrees of freedom information.

Nevertheless, more than one DRF may be provided if a selected type of motion is not fixed or trackable. For example, a rotational movement may not be fixed and therefore at least one degree of freedom, or one type of motion may not be tracked by the tracking system. Therefore, it may be selected to include more than one DRF to

allow for determination of the type of movement not detectable by the single DRF but may be compared between a plurality of the DRFs to determine the last type of motion. Alternatively, the single DRF may only include two orthogonal coils and still be rotationally fixed to the patient. However, use of the two coils generally will not provide 6 degrees of freedom information.

In this regard, generally in an electromagnetic tracking system, three coils substantially unaligned with one another, such as orthogonal to one another, are required to provide six degrees of freedom information. These coils or tracking sensors may be located in a single DRF. Alternatively, three DRFs, where each DRF includes a single coil, where each coil is again not positioned coaxial or linear relative to the other coils. This combination will also provide six degrees of freedom information. By providing less than three coils within a single DRF enables the DRFs to be smaller due to requiring less coils and hence, overall smaller size. Therefore, a single six degree of freedom DRF would generally be larger than individual DRFs each providing only a single coil and three degrees of freedom information. The size of the DRFs may assist in positioning the smaller DRFs relative to a selected portion of the anatomy. This may be useful when positioning the smaller DRFs in substantially tight or small areas, such as under a small tissue portion relative to the cranium or any selected portion of the anatomy, such as cervical vertebrae. Nevertheless, the smaller DRFs would be used for any appropriate purpose.

With reference to FIG. **19**, a tracking sensor that can also operate as a DRF **350** is illustrated. The DRF **350** generally includes a tracking sensor that can be tracked with a tracking system. The DRF **350** may be positioned relative to a bone or anatomical portion **352**. The bone may be any appropriate bone, such as a femur, humerus, etc. For example, a bore **354** may be formed in the bone **352** to receive at least a portion of the DRF **350**. The DRF **350** may include a wired portion **356**, which may provide power to the DRF **350** or transmit a signal from the DRF **350**. It will be understood, however, that the DRF **350**, or any appropriate DRF discussed above or herein may be substantially wireless. For example various wireless channels may be used to transmit or receive information. Various internal power sources may be provided, such as an internal battery. A power signal may be used to apply remote power to the DRF, and an LC Tank circuit may be used to transmit a signal. Various exemplary wireless DRFs are described in U.S. patent application Ser. No. 10/245,843, entitled, "SURGICAL COMMUNICATION AND POWER SYSTEM", filed Sep. 22, 2002; and U.S. patent application Ser. No. 10/837,997, filed May 3, 2004, entitled, "METHOD AND APPARATUS FOR IMPLANTATION BETWEEN TWO VERTEBRAL BODIES", each of which is incorporated herein by reference. The DRF **350** may be any appropriate sensor, such as an acoustic sensor, an optical sensor, an electromagnetic sensor, or a combination thereof. Regardless, the DRF **350** may be positioned in the bore **354** to substantially receive the DRF **350**, such that it can be fixed relative to the bone **352**.

Positioning the DRF **350** in the bore **354** may eliminate or reduce the need for other attachment mechanisms to provide for a fixed position of the DRF **350** relative to the bone **352**. For example, various pins, interference portions, and the like may be used to interconnect the DRF **350** with the bone **352**. For example, various screws, pins, interference portions, and the like, may be provided and connect the DRF **350** with the bone **352**. Also, in addition to or alternatively to the pins, the DRF **350** itself may be formed in an interference shape such as a square, polyhedron, etc. The various geometries may

interact with the bore 354 to resist or eliminate rotation of the DRF 350. Nevertheless, the use of the bore 354 may assist in assuring the DRF 350 does not move relative to the bone 352, whether or not various other interconnection portions are used. It will be understood, however, that the bore 354 may both fix and reduce an exposed profile of the DRF 350.

Further, it will be understood that the DRF 350 need not include the wire 356. For example, the DRF 350 may be substantially self-powered or powered by an external source or signal. Therefore, the wire 356 may not be necessary and the DRF 350 may be provided in the bore 354 alone.

In addition, the bore 354 may allow the DRF 350 to be positioned relative to the bone 352 and be provided below or underneath a surface of soft tissue 360. Therefore, the DRF 350 may be a substantially sub-dermal or sub-soft tissue DRF. This may allow the DRF 350 to be positioned in the bone 352 and remain in the bone 352 while not affecting a soft tissue 360 that may be positioned next to the bone 352. This may also assist in providing a substantially normal operation, such as a range of motion, of the bone 352 with the soft tissue 360 in place. In this case the profile or shape of the DRF 350 may be made to reduce or eliminate any sharp edges or surfaces to prevent the DRF 350 from interfering with the soft tissue 360.

Nevertheless, as discussed above, the DRF 350 may be tracked according to various procedures to allow for a determined position of the DRF 350. Therefore, movement of the bone 352 may be tracked with the DRF 350 even while soft tissue portions, such as the soft tissue 360, surrounds or is positioned relative to the bone 352. Keeping or positioning the soft tissue 360 near the bone, in a generally natural orientation, may allow for obtaining a substantially natural motion of the bone 352.

With reference to FIGS. 20-24, various DRFs according to various embodiments, may include mechanisms to reduce rotation or other unselected movement of the DRF relative to a selected portion, such as a portion of the anatomy. Further, it will be understood that the DRF sensor, as a part of the DRF, may be positioned at any appropriate position relative to the anatomy or any other portion to which it is fixed. Therefore, it will be understood that DRFs, according to the various embodiments may include mechanisms or apparatuses that fix the DRF in a selected orientation or position relative to an anatomy, or other appropriate portion.

Various DRFs according to various embodiments, may include the DRF or DRF assembly 370, illustrated in FIG. 20. The DRF 370 may include a DRF sensor portion 372 that may be a substantially optical DRF, an electromagnetic DRF, and acoustic DRF or the like. Nevertheless, the DRF sensor 372 may be provided with the DRF 370 in a substantially anti- or reduced rotation mechanism. The DRF sensor 372 may include a wired portion 374, as discussed above. Nevertheless, also as discussed above, the DRF sensor 372 may be substantially wireless and include a power signal or be internally powered, such as those discussed above.

The DRF sensor 372 may be attached to a connection portion 376 that includes a first arm or leg 378 that is hingedly or movably interconnected with a second arm or leg portion 380. The first leg portion 378 may be movable relative to the second leg portion 380 with a movement mechanism 382. The movement mechanism 382 may be any appropriate mechanism, such as a screw that interconnects a boss 384 extending from the first leg 378 with the second leg 380. Therefore, movement of the screw 382 may move the first leg 378 relative to the second leg 380. In this way, the

two legs 378, 380 may be moved and locked or fixed relative to one another to form an engagement relative to a selected surface, such as a spinous process of a vertebra of the spine. In addition, the legs 378, 380 may include further engagement portions 386 that assist in holding the DRF 370 relative to a selected position. For example teeth or spikes may be included as the engagement portions 386 to bite into or fixedly engage the anatomy, such as a spinous process S. In addition, the screw 382 may be operated with any appropriate mechanism, such as with a tool, substantially manually operated, or the like.

Nevertheless, the DRF 370 may be positioned relative to a selected portion of the anatomy, substantially in a manner that reduces or eliminates rotation of the DRF 370. As discussed above, various degrees of freedom of the DRF 370 such as six degrees of freedom (6 DOF), to assist in determining its location, may be determined using various techniques. The accuracy or efficacy of the determined locations may be reduced if the DRF 370 is allowed to rotate relative to a selected portion. Therefore, various mechanisms, such as the first leg 378 and the second leg 380 that may be positioned relative to one another, may assist in reducing or eliminating the rotation of the DRF 370. Fixing rotation of the DRF 370 may assist in assuring that substantially any movement of the DRF 370, such as the DRF sensor 372, may be due to the portion to which the DRF 370 is attached and not to motion of the DRF 370 itself.

With reference to FIG. 21, a DRF or DRF assembly 400 is illustrated. The DRF assembly 400 may include a DRF sensor 402, a DRF connection portion or anti-rotation portion 404 and an interconnection portion or member 406. Generally, the DRF sensor 402 may include a casing that surrounds the sensor portions of the DRF sensor 402. Nevertheless, the interconnection portion 406 may include a shaft 408 defining a thread 410. The thread may engage a portion of the connection member 404 as to substantially fix the DRF sensor 402 relative to the connection portion 404. The connection portion 404 may also include a first leg 412 and a second leg 414. The two legs 412, 414 may engage two sides of a selected structure, such as a spinous process S of the spine (FIG. 21A). In the case of engaging a spinous process, the threaded portion 410 may both engage one or both of the spinous process and the connection member 404.

Regardless, the interconnection with the connection member 406 may assist in holding the connection member 404 relative to the selected portion of the anatomy. The two legs 412, 414 may allow for at least two points of contact to resist movement of the DRF sensor 402, such as rotational movement thereof, relative to a structure of the anatomy. Therefore, the DRF 400 may be positioned relative to a portion of the anatomy while substantially reducing a selected motion of the DRF 400 relative to the anatomy. As discussed above, position information of the DRF 400 may be used to determine a location of a selected portion of the anatomy, such as a spinous process or a vertebra.

As exemplary illustrated in FIG. 21A, each of the legs 414, 412 may engage or contact a selected side of the spinous process S. The legs may further include engagement portions to bite into or fixedly engage the spinous process S. Further, the screw may be screwed into the spinous process to lock or fixedly engage the DRF 400 together. The screw may engage the sensor portion 402 relative to the member 404 to hold the sensor 402 in a selected position. Also the sensor 402 may be keyed, such as with the member 404, such that it may not rotate relative to the legs 412, 414.

With reference to FIG. 22, according to various embodiments, a DRF or DRF assembly 430 is illustrated. The DRF

assembly **430** may include a DRF sensor portion **432**, which may include or provide a DRF sensor. The DRF sensor may be any appropriate tracking sensor, such as an optical sensor, an acoustic sensor, an electromagnetic sensor, or any appropriate sensor. The DRF assembly **430** further includes an engagement portion or member **434**, such as a member to engage a selected portion of the anatomy. A further connection portion **436** is provided to interconnect the DRF sensor **432** with the connection member **434**.

The interconnection portion **436** may include a shaft **438** that defines a thread **440**. The shaft **438** may pass through a bore **442** formed in the sensor portion **432** to engage or pass through the attachment member **434** and engage a selected portion of the anatomy, such as a bone. In addition, the connection portion **436** includes a surface or structure **444** that may interconnect or mate with a second surface or structure **436** defined by the connection portion **434**. Therefore, the DRF sensor **432** may be held fixed relative to the connection portion **434** in a selected manner and/or orientation. Further DRF sensor **432** may be keyed or include portions to engage the member **434** to resist or eliminate rotation relative to the member **434**.

In addition, the connection member **434** may include a first leg portion **448** and a second leg portion **450** that may allow for at least two points of contact with a selected portion. For example, the two portions **448**, **450** may engage either side of a spinous process to assist in holding the DRF assembly **430** relative to the spinous process, for example similar to the legs **412**, **414** in FIG. 21A. The portions **448**, **450** may assist in reducing or eliminating rotation of the DRF assembly **430**, including the DRF sensor **432**, relative to the anatomy or other structure. Therefore, the threaded portion **440** may engage a portion of the anatomy compressing the connection portion **436** to interconnect the first structure **444** with the second structure **446**. In addition, the first portion **448** and the second portion **450** may engage two sides or two points relative to a selected portion of the anatomy for assisting and holding the DRF assembly **430** relative thereto in a substantially immovable manner.

As discussed above, the DRF assembly **430**, including the DRF sensor **432**, may assist in determining a position of the DRF assembly **430** and a portion to which it is interconnected. Therefore, reducing a motion of the DRF sensor **432** relative to a selected member may increase the accuracy, the efficacy and the degrees of freedom of the sensed movement or position of the member to which the DRF assembly **430** is attached.

With reference to FIG. 23, a DRF assembly **460** is illustrated. The DRF assembly **460** may include a first portion **462** that may define or include a DRF sensor **464**. As discussed above, the DRF sensor **464** may be any appropriate sensor, such as an optical sensor, an acoustic sensor, an electromagnetic sensor, or combinations thereof. Similarly, as discussed above, the DRF sensor **464** may be substantially wired or wireless according to various embodiments.

The first portion **462** may extend or be interconnected with a second portion or shaft portion **466**. The first portion **464** may be substantially fixedly attached to the shaft portion **466** or may be removable therefrom. The shaft portion **466** may extend from a base portion **468** that is operable to interconnect with a selected member, such as a portion of the anatomy including a cranial or spinal region. Therefore, the shaft member **466** and/or the base member **468** may be implanted at a selected time and the first portion **462** may be interconnected with the shaft **466** at a selected later time. Further, it will be understood that the shaft **466** and/or the base **468** may be provided as fiducial markers. These por-

tions may be inserted as markers for use in pre-operative imaging and used as fiducial markers for registering the images before or after the DRF **462** is attached.

The base portion may include one or a plurality of anti- or reduced rotation members **470**. The anti-rotation members **470** may engage a member, such as an anatomical structure, including a bone, off center from a central axis defined by an attachment mechanism **472**, such as a screw. The screw **472** may interconnect the base **468** with a selected portion of the anatomy, while the anti-rotation pins **470** interconnect the base **468** with the anatomy at a different axis. Therefore, rotation around the axis of the screw **472** may be substantially reduced or eliminated. It will be understood that a plurality of the anti-rotation pins **470** may be provided according to various embodiments.

Also, the shaft **466** may be provided in a plurality of lengths depending upon various applications. For example, the shaft may include a length of one centimeter or less for various low profile or percutaneous applications. Other applications may use a longer shaft, such as a shaft greater than about one or two centimeters for various applications, such as connection to a spinous process or a cranial portion. Regardless, the anti-rotation pins **470** may assist in eliminating rotation of the first portion **462**, including the DRF sensor **464** relative to a selected portion of the anatomy, such as a bony portion.

In addition to the anti-rotation pins **470**, or alternatively thereto, the base **468** may also define a spike or projection **474**. The spike **474** may engage the member, such as a bony structure at an axis different from the axis of the screw **472**. The spike may also assist in reducing rotation or rotational tendencies of the DRF assembly **460**.

The spikes **474** may be molded into the base **468** to first engage a selected portion, such as a bony portion. After preliminary engagement, the separate of modular anti-rotation pins **470** may be passed through the base **468** to further assist in reducing rotation of the DRF assembly **460**. Therefore, it will be understood that the DRF assembly **460**, or any appropriate DRF assembly, may include one or a plurality of anti-rotation mechanisms.

With reference to FIG. 24, a DRF assembly **490** according to various embodiments is illustrated. The DRF **490** may include a body portion **491** defining a first leg **492** and a second leg **494**. A connection mechanism **496** is provided to interconnect the DRF **490** with a selected portion, such as a portion of an anatomy.

The connection mechanism **496** may define a thread **497**. The thread **497** may engage threads defined by the body **491**. The connection mechanism may further engage the anatomy. Also, the legs **492**, **494** may include a structure **498** operable to engage a portion of the anatomy. A spike or further fixing member **499** may extend from the legs **492**, **494** to engage the anatomy.

The connection mechanism **496** may be used to connect the body **491** to the anatomy. As discussed above, according to various embodiments, each of the legs **492**, **494** may engage a different portion of the anatomy to resist rotation or other movement of the DRF **490**. This may hold a DRF sensor portion in a selected position relative to the anatomy. The DRF sensor portion may be included in the body **491**, the connection mechanism **496**, or connected to either. For example, after positioning the DRF assembly **490**, a DRF sensor may be fit to the connection mechanism **496**.

It will be further understood that a DRF or other instrument may include one or a plurality of anti-rotation mechanisms according to various embodiments. Therefore, the DRF need not include only a single or small combination of

anti-rotation mechanisms, but may include a plurality of more than one anti-rotation mechanism. Further, as briefly discussed above, various anti-rotation mechanisms may be selected based upon various applications. For example, a DRF to be interconnected with a spinal portion, such as a spinous process, may include various anti-rotation mechanisms, while various other DRFs may include different anti-rotation mechanisms.

With reference to FIG. 25A, an instrument 520 that may include a tracking sensor 522 is illustrated. The tracking sensor 522 may be positioned in any appropriate position, such as in a handle portion 524. The tracking sensor 522 allows the instrument 520 to be tracked such that a location of the instrument 520 or a member to which is connected can be tracked. The tracking sensor 522 may be any appropriate tracking sensor, such as an electromagnetic sensor, an optical sensor, an acoustic sensor, or the like. Nevertheless, the tracking sensor 522 may be positioned in the handle 524 or any appropriate portion relative to a shaft or extension portion 526.

The shaft 526 may include a fitting or connection end 528. The connection end 528 may include a locking or spring paddle portion 530. The attachment portion 530 may include a flexible or deformable member 532 that may flex or move relative to the shaft 526 through a flexing or hinge area 534. The inner connection portion 530 may allow the instrument 520 to be interconnected with a selected instrument or tool, such as a cutting block 540 (FIG. 26), in a desired orientation.

The tracking sensor 522 interconnected in the instrument 520 may be used to sense a position of the instrument 520 relative to the tool 540. For example, the length of the shaft 526 or an orientation of the shaft 526, may be known relative to a selected portion of the shaft, such as the interconnection portion 530. Thus the location and orientation of the tracking sensor 522 relative to the tool 540 is known. This known orientation and location can be used to assist a user, such as a surgeon, in a procedure, such as an orthopedic procedure. For example, the tool 540 may be a cutting block to be oriented for a selected resection.

With reference to FIG. 25B, an instrument 520' may include a shaft 544 that includes a bent or angled portion 546. The instrument 520' may still include the tracking sensor 522 in the handle or operable portion 524 for positioning or operating the instrument 520'. Further, the instrument 520' may include an attachment region 530 similar to the attachment region 530 of the instrument 520'. The bent portion 546, however, may allow for positioning of the instrument 520' in a selected position that may not allow for a substantially straight shaft. In addition, the bent shaft 544 may allow for an efficient use of the instrument 520', such as easy viewing of a surgical area or movement of selected instruments, such as a minimally or less invasive surgical procedure.

Regardless of the configuration selected for the shaft 526 or any appropriate shaft portion, such as the shaft 544, the instrument 520 may be fit relative to the tool 540 that may be a cutting block, as illustrated in FIG. 26. For example, to resect a selected portion of anatomy, such as a tibia 550, the cutting block 540 may be positioned relative to the tibia 550. The cutting block 540 may be held relative to the tibia 550 in any appropriate manner. For example, a pin 552 or a plurality of pins 552 may be provided to fix the cutting block 540 in a position relative to the tibia 550.

In a surgical navigation system, such as the system described above, it may be desirable to assure that the cutting block 540 is positioned at a selected position, ori-

entation, etc. The instrument 520, including the interconnection portion 530, may be positioned relative to the cutting block 540. For example, the cutting block 540 may include a guide or cutting slot or surface 554 defined by the cutting block 540. The interconnection portion 530 of the shaft 526 may be fit into the guide slot 554 to hold the instrument 520 relative to the cutting block 540. It will be understood that the interconnection region 530 may be any appropriate interconnection region and is not limited to a spring member 532. For example, various deformable legs, quick-release screws, and the like may be used to efficiently interconnect the instrument 520 with a selected member.

Once the instrument 520 has been fit in the cutting block 540 the tracking sensor 522 may be used to determine a location and orientation of the guide slot 554 of the cutting block 540. This may assist in insuring that the cutting slot or guide surface 554 is positioned relative to the tibia 550 in a selected position, such as a pre-selected or planned position.

Therefore, the instrument 520 may assist in positioning or determining a position of the cutting block 540 relative to a selected portion of the anatomy. This may also allow a user to determine a cutting plane and the cutting plane may be displayed for use by a user. The instrument 520 may be used without pre-selecting or knowing the position or type of cutting block 540. Thus any appropriate cutting block 540, or other tool, may be used with the instrument 520 to ensure a proper or planned location, orientation, angle, etc. is obtained without including the tracking sensor 522 on the tool 540.

The instrument 520 may be inserted into the tool 540 before fixing the tool relative to the patient, as well. This may allow a representation of the tool 540 to be displayed relative to the patient 14 on the display. This may allow the tool 540 to be positioned in a substantially planned or selected position, for example in a less or minimally invasive procedure. The user may use the display with the represented tool 540 to ensure that the selected location, orientation, etc. is achieved before or while fixing the tool to the patient or using the tool 540. Also, the plane of the cut may be displayed on the display 36 prior to the cut being formed.

It will be understood that the instrument 520 may be used with any appropriate tool, such as a cutting block for cutting various other portions of the anatomy, other than the tibia 550. For example, the interconnection region 530 may be interconnected with the cutting block for selecting a cut in a spinal area. In addition to determining the position of the cutting slot 554, or any appropriate cutting slot, the instrument 520 may be used to determine an orientation of the cutting guide 554 relative to a selected surface. For example, as discussed above, the tracking sensor 522, may be used to determine an angle of a selected portion, such as the cutting guide 554, relative to the anatomy. Further, the instrument 520 may be used to determine a depth or length to be formed with the guide 540.

In addition, the interconnection region 530 allows for a substantially efficient connection of the instrument 520 to a selected portion, such as the cutting block 540. As discussed, the connection portion 530 may be any appropriate interconnection region 530. For example a screw, a pin, or the like may be used. Regardless, the instrument 520 may allow for the navigation of the tool 540 without including a sensor on the tool 540. Thus, the tool 540 need not include the bulk of the sensor or be specially made to include the sensor for use with the tracking system 44.

The interconnection portion 530 may allow for a hands-free or single hand operation of the instrument 520. Once

positioned, the instrument **520** may be held relative to the cutting block **540** with no additional need for intervention by a user. Therefore, the instrument **520**, including the tracking sensor **522**, may be positioned in a selected cutting block and held in the selected cutting block with the interconnection region **530** for various procedures. Also, the position of the cutting block **540** can be determined with the instrument **520** by positioning the instrument **520** and using the navigation system **10**.

Regardless, the instrument **520** may be efficiently connected with an instrument or tool for determining a location of the tool. A user need not hold or continually hold a probe relative to a tool when the instrument **520** may be interconnected with the instrument for a selected period of time. Therefore, the cutting block **540** need not permanently include a separate or its own tracking sensor, but may use the tracking sensor **522** interconnected with the instrument **520** for locating and tracking purposes.

Further, as discussed above, the instrument **520** may include the angled shaft **544** or straight shaft **526**. It will be further understood that a plurality of shafts, including various angles, lengths various configurations or geometries, or the like, may be provided. Each of the plurality of shafts, including a selected feature, may be interconnected with a single handle portion **524**, which may include the tracking sensor **522**. Therefore, an inventory or kit may be maintained of the plurality of the shafts **526**, **544** without providing a plurality of the tracking sensors **522**. Further, various or all portions of the instrument **520** may be reusable or disposable. For example the shaft **526** may be substantially disposable and the handle **524** may be reusable and or can be sterilized. It will be understood, that this is merely exemplary and any portions maybe disposable or reusable. Moreover, the sensor **522** may be wired or be wireless, such as that described above.

Although the instrument **522**, which may include the tracking sensor **522**, may be provided to be interconnected with the tool **540**, it will be understood that the tool **540** may also include integrated tracking sensors. Therefore, although the instrument **520** may be interconnected with the tool **540** to assist in planning or tracking the position of the tool **540** relative to a selected portion, such as the tibia **550**, the tracking sensor **522** may not be provided in the instrument **520**, but may be included in the tool **540**.

Including the tracking sensor **522**, or any appropriate tracking sensor in the tool **540**, may assist in minimizing the size of the tool **540** or the portion required to track the tool **540**. Therefore, a position, orientation, or the like of the guide surface **544** of the tool **540** may be determined relative to the anatomy, such as the tibia **550**. This may allow for tracking a tool or a position of the tool **540** relative to the anatomy for a selected procedure. Further, the tool **540**, if it includes the tracking sensor, or is used with the instrument **520**, may be used to achieve a planned procedure. Therefore, it will be understood that the tool **540** or any appropriate tool may include integral tracking sensors rather than providing the instrument **520** separate or interconnectable with the tool **540**.

With reference to FIG. 27A, a DRF or a low profile DRF assembly **560** is illustrated. The DRF **560** may include a case or assembly housing **562** that surrounds one or more DRF sensors or coils **564a**, **564b**, **564c**, for various purposes, such as those described herein. As discussed above, the DRF **560** may be any appropriate DRF, such as an acoustic DRF, an electromagnetic DRF, or an optical DRF. Nevertheless, as discussed above, the DRF sensors **564** may include electromagnetic coils or coils that may sense a position in electro-

magnetic field, such that a direct line of sight between the DRF sensor **564** and a receiver or localizer is not necessary. Therefore, the housing **562** may include a size that allows it to be positioned within a selected portion of the anatomy, as discussed herein.

For example, the DRF housing **562** may include a height that is less than about two centimeter or a height that is less than about one centimeter. It will be understood that the height of the DRF case **562** may be any appropriate height to allow it to be positioned relative to a selected portion of the anatomy. The case **562** may also include a shape or geometry that allows a substantially smooth movement relative to soft tissue of an anatomy, such as when the DRF **560** is positioned subdermally. Thus the size and geometry of the case **562** may provide for a subcutaneous placement and movement of the DRF **560**. The shape allowing for the subcutaneous placement may be substantially short, such as less than about 2 cm. Also the shape may be substantially smooth to allow the soft tissue to move over a surface of the DRF **560**. This allows the DRF **560** to be positioned and allow soft tissue to move relative to the DRF **560** without the DRF **560** substantially interfering with the movement of the soft tissue.

The DRF **560** may be positioned relative to a portion of the anatomy, such as a soft tissue portion or bone portion with a connection mechanism, which may include a screw **566** or a plurality of screws **566**. In addition, as discussed above, the DRF **560** may include anti-rotation or fixation portions **568**. The anti-rotation or anti-movement portions **568** may extend from a surface, such as a bottom surface **562a** of the DRF case **562**. The anti-rotation portions **568** may engage any appropriate portion, such as a bony surface, a soft tissue portion, or the like to assist in holding the DRF **560** or the DRF sensors **564** in a selected location.

In addition, the DRF sensor **560** may be provided, such that it may be moved relative to the soft tissue and then held in a selected position. Therefore, the DRF case **562** may include substantially soft or smooth sides that do not include sharp edges, such as would be found in a square or other angular geometry. Nevertheless, it will be understood, that the DRF case **562** may be provided in any appropriate shape or size.

With reference to FIG. 27B, a low profile DRF **560'** is illustrated. The low profile DRF **560** may be similar to the low profile DRF **560'** illustrated in FIG. 27A. The low profile DRF **560'**, however, may include only a single or a plurality of the screws **566** or a single or plurality of the spikes **568**. The spike **568** may act as an anti-rotation device such that the low profile DRF **560'** does not move or rotation relative to an axis thereof. It will be understood that the low profile DRF **560'** or any DRF according to various embodiments, generally may include at least two points of contact with a selected anatomical portion to substantially reduce or resist rotation of the DRF. Therefore, the low profile DRF **560'** or a DRF according to any appropriate embodiment may be interconnected with a portion of the anatomy for assisting in obtaining and maintaining registration of image space to patient space and the DRF may maintain the registration by reducing or eliminating error due to rotation. Therefore, the DRFs according to various embodiments, such as the low profile DRF **560'**, may include a mechanism to create two points of contact with the selected portion of the anatomy rather than a plurality more than two contacts.

The DRF **560**, according to various embodiments, may be provided with various types of screws **566**. For example, the screws **566** may be substantially self-tapping, drill tapping or any appropriate type of screw. Therefore, the screw **566**

may be positioned in a portion of the anatomy, such as bone, in a preformed hole or a hole that is tapped by the screw **566**.

Further, the screw **566** may be inserted in any appropriate manner. For example, the screw **566** may be captured in or held relative to any driver to assist in driving the screw **566** relative to the DRF **560**. The screw may be captured relative to the driver using a tapered fit or other type of interference fit between the screw and the driver. Therefore, the screw may be held relative to the driver, such that a generally one handed driving may occur. The driver may be interconnected with a power drill or may be hand driven for inserting the screw relative to the anatomy through the DRF **560**. Further, the screws **566** may be captured in the DRF **560**, such as in the body **562**. For example, the bores or holes, through which the screws **566** pass, may include a locking or capturing tab to allow the screw **566** to be held relative to the DRF for a selected period of time.

Further, it will be understood that the screws **566** may include any appropriate driving form. The driving head of the screw **566** may include a cruciform driving mechanism, a box, or square driving mechanism, a hex driving mechanism, or any appropriate type of mechanism. Further, the driving head may assist in holding or aligning the screw relative to the driver to assist in positioning the screw relative to the DRF **560**.

Further, the DRF **560** or DRF according to any appropriate embodiment, may include a body **562** that is substantially deformable or conformable. For example, the body **562** may include a substantially flexible body or material that allows the body **562** to conform to the surface onto which it is placed. For example, such as the DRF described above in FIG. **3**, the DRF may include a portion that is flexible that engages the anatomy. Therefore, the DRF may substantially conform to the anatomical structure to assist in holding the DRF in a selected position. The body **562** may be deformed with exterior pressure or when positioning the screws **566**, or any appropriate holding mechanism, relative to the anatomy.

Although the body **562** may be flexible to assist in positioning the DRF **560** relative to the anatomy. The tracking sensors **564A-564C** of the DRF **560** may be tracked by the tracking system in any appropriate manner. For example, the tracking sensors **564A-564C** may be positioned within a substantially rigid portion of the body with the body **562** being deformable relative to the rigid portion holding the tracking sensors **564A-564C**. In this way, the tracking sensors **564A-564C** are held fixed relative to one another to maintain registration of the DRF **560** relative to a portion of the anatomy. Alternatively, or in addition thereto, the body **562** may be substantially completely flexible such that the tracking sensors **564A-564C** of the DRF **560** are able to move relative one to another during the deformation or confirmation of the body **562**. In this case, registration is performed after the DRF **560** is securely fixed to the patient in its conformed condition.

Regardless, the DRF **560**, or a DRF according to any appropriate embodiment, may include a body or structure that is able to conform to a selected portion of the anatomy. The deformation or confirmation of the body **562** or any appropriate body may assist in holding the DRF relative to the selected portion of the anatomy during a selected period of time. For example, although the DRF may be provided with a substantially planar bottom **562A**, it may be positioned relative to a non-planar surface and deformation of the body **562** to conform to the non-planar surface may assist in positioning or holding the DRF **560** relative to the selected portion of the anatomy.

According to various embodiments DRFs, such as the DRF **560** may be used to position relative to soft tissue. As discussed above and herein a DRF may be positioned relative to or in soft tissue and not obstruct movement of the soft tissue or other anatomical portions. With reference to FIGS. **28A-28C** an exemplary method is illustrated.

With initial reference to FIG. **28A** an exemplary incision **574** may be made through a selected portion of soft tissue, such as dermis, skin, fascia, muscle, or any appropriate portion. The incision **574** may be used for performing a selected procedure, such as those discussed above and herein. Nevertheless, it may be selected to position the DRF **560** at a location M not at the location of the procedure. Thus the incision **574** may be moved in direction of arrow N towards the selected location M.

Once at the selected location M, illustrated in FIG. **28B**, the DRF **560**, or any appropriate DRF, may be positioned. The DRF **560** may be fixed to bone, soft tissue, or any appropriate portion. Once the DRF **560** is positioned at the selected location M the incision **574** may be moved back to its initial position, near where the procedure is to be performed, FIG. **28C**. As discussed above this may allow a transdermal or sub-dermal placement of the low-profile DRF **560**, or any appropriate DRF. The DRF **560** may be provided with a selected size or shape, such as a low profile (such as less than or equal to about 2 cm in height), to allow for movement of the incision after placing the DRF **560**.

Thus the single incision **574** may be used to both position the DRF **560** and perform a selected procedure. This may reduce incisions to be formed and decrease recovery time for the patient **14**. Thus, the incision **574** may be formed at a first location, the DRF **560** positioned, through the incision **574**, at a second location, and the incision returned to a third location, which may be the first location. The sub-dermal placement may assist in performing minimally or less invasive procedures, such as minimally invasive orthopedic procedures.

According to various embodiments, with additional reference to FIG. **28D**, a portion of an anatomy, such as a leg **572** may exemplarily have a procedure performed relative thereto. For example, an incision **574** in a soft tissue **576**, such as skin or muscle surrounding a selected portion, such as a femur **578**, may be provided. The DRF **560** may be positioned relative to a portion of the anatomy, such as the femur **578**. The DRF **560** including a selected size, such as less than about one centimeter in height, may be positioned or fixed relative to the femur **578**.

After positioning the DRF **560** relative to the femur, the incision **574** may be unretracted or placed over the DRF **560**. For example, a retractor **580** may be used to move a portion of the soft tissue or expand the incision **574** for positioning of the DRF **560** on a particular portion of the femur **578**. After positioning the DRF **560** relative to the femur **578**, the retractor **580** may be removed and the soft tissue allowed to be replaced or moved back over the DRF **560**.

Once the soft tissue is positioned over the DRF **560**, various tracking or localization procedures may be used to determine a position of the DRF **560** and further determine a position of the femur **578** relative to other portions. For example, a second DRF **582** may be positioned relative to a tibia **584**. Therefore, the DRF **560** may be used to determine a location of the femur **578** relative to the second DRF **582** and the tibia **584**. The size, shape, orientation, and other features of the DRF **560** may allow the DRF **560** to move relative to the soft tissue **576** surrounding the DRF **560**, after the soft tissue is replaced, and the femur **578**. This may be useful in determining a range of motion of the femur **578**.

relative to the tibia **584**. It will be understood that a range of motion of any two bones relative to a joint may be determined using the DRF **560** and any other appropriate DRF portions, such as the second DRF **582** or a second of the DRFs **560**.

A range of motion may be determined after resurfacing a bone surface or positioning an implant relative to a bone. The range of motion may assist in determining a proper placement of a prosthesis or an appropriate resection or resurfacing of a bony portion. Therefore, allowing the DRF **560** to move with a bone portion, such as the femur **578**, with the soft tissue in a substantially natural position, may assist in determining a proper conclusion of a procedure.

Further, it will be understood that the DRF **560** need not be fixed directly to a bony portion. For example, the DRF **560** may be interconnected with a selected portion of soft tissue, such as a muscle, a tendon, a ligament, or any other appropriate soft tissue portion. The DRF fixed to a selected soft tissue portion may move with the soft tissue portion relative to other portions of the anatomy or other instruments. Regardless, movement of the soft tissue may be determined by use of sensing the location of the DRF **560**, as discussed above.

Again, the DRF **560** may be provided in an appropriate size, geometry, location and the like to allow it to move relative to soft portions of the anatomy. The features of the DRF **560** may allow it to not obstruct the movement of the soft tissue to which the DRF **560** is attached or the soft tissue relative to which the DRF **560** is moving. Thus, the DRF **560** may be positioned and used to determine a movement of a bony portion, a soft tissue portion, and the like, where the DRF is moving and touching the soft tissue portions without interrupting the movement of the various selected portions. It will be understood that the DRF **560** may be any appropriate size, or any appropriate DRF. The DRF **560**, or any appropriate DRF, according to various embodiments, may include selected sizes, shapes, and/or configurations to assist in movement relative to various selected locations. For example, the percutaneous or subcutaneous placement of the DRF may be performed without requiring an external positioning or fixation of the DRF. Further, the DRF **560** may be substantially wired or wireless to allow for various configurations and purposes.

With reference to FIGS. **29** and **30**, a mobile localizer **600**, according to various embodiments, is illustrated. The handheld or mobile localizer **600** may be similar to the transmitter coil array **46** and may be part of the electromagnetic navigation or tracking system **44**. The mobile localizer **600** may be used in conjunction with or in addition to the coil array **46**. The coil array **46** may be used to form a field until an obstruction is positioned that distorts the field and then the mobile localizer **600** may be used. Alternatively, both may be used together to assist in determining a location of the tracking sensor.

It will, nevertheless, be understood that the mobile localizer **600** may be an instrument separate from the tracking system **44**, but may include portions or control systems similar to the tracking system **44**. The handheld localizer **600** may include portions similar to the transmitter coil array that allows for localization, registration, and the like of various portions, such as the DRF **54**, any appropriate DRFs, such as those discussed above, the probe or pointing device **66**, or any appropriate member.

The mobile localizer **600** may include any appropriate shape, size, geometry, and the like according to various purposes. For example, the mobile localizer may include a first lobe or portion **602**, a second lobe **604**, and the third

lobe **606**. Each of the lobes **602**, **604**, **606** may house or define a transmitter coil positioned or included in the mobile localizer **600**. It will be understood that the mobile localizer **600** may include a substantially round, square, rectangle, or any appropriate shape. The lobe shape is merely exemplary and not limiting.

Further, the mobile localizer **600** may include a power and/or transmission cable **608** interconnected with a selected power source and/or tracking system. For example, the cable **608** may interconnect the mobile localizer **600** with the coil array controller **48** for transmission and/or reception of a tracking signal. The mobile localizer **600**, therefore, may be used to communicate or be operated by the system **44** to assist in tracking or locating a selected sensor, such as the DRF **54**. It will be understood, however, that the mobile localizer **600** may also be internally power or powered with a power signal. The mobile localizer may also include a wireless transmitter or receiver. This may allow the mobile localizer to be substantially wireless.

Further, a handle or graspable portion **610** may extend from a housing **612** defining the selected instrument. The graspable portion **610** may be used to orientate or move the mobile localizer **600** relative to a selected portion, such as the patient **14**. It will be understood, however, that the mobile localizer **600** need not include a graspable portion **610**. A user, such as a physician may grasp the mobile localizer **600** directly. Also the mobile localizer **600** may be substantially wireless.

The mobile localizer **600** may include the casing **612** that is easily removable from the various coils held within the lobes **602**, **604**, **606**. The casing **612** may be substantially sealable relative to a selected external environment, such that a casing **12** may be easily sterilized and replaced over the coils. The case **612** may also be disposable and discarded after a use. Alternatively, or in addition to the casing **12**, a sterile bag **616** may be provided to selectively surround a portion of the mobile localizer **600**. Therefore, the mobile localizer **600** may be used in a sterile environment through a plurality of applications without contaminating the sterile environment. It will be understood that any appropriate sterilization technique or portions may be used to insure a sterile environment for the mobile localizer **600**.

The mobile localizer **600** may include any appropriate selected dimensions. For example, the mobile localizer **600** may include external dimensions of about 50 cm². It will be understood, however, that the mobile localizer **600** may include any appropriate dimensions, such as less or more than about 50 cm². Regardless, the mobile localizer **600** may be moved by the physician or user **614** to any appropriate location relative to the patient **14**.

With reference to FIG. **30**, the mobile localizer **600** may produce a field LF that can be selectively directed over a selected area, such as a surgical area SA. The field LF, as discussed herein may be tuned or shaped for various reasons using various components and coil orientations. Further size of the field may be selected depending upon a size of the mobile localizer **600** and may be any appropriate size. Also the coils included in the mobile localizer **600** may be of a selected size to assist in selecting a size or strength of the field LF. Thus the mobile localizer **600** may include various dimensions, such as a selected area or face **601** or volume (such as a three dimensional size). The area **601** may be an area through which the field LF is focused or directed while a volume may be a three dimensional size of the mobile localizer **600**. The mobile localizer **600** may also include a mass of less than about 2 kg, and may even be smaller than about 1 kg.

The mobile localizer **600** may include coils of any selected size. The coils, however, may be larger, and may be similar in size to coils used in the coil array **46**. Nevertheless, the coils in the mobile localizer **600** may be positioned in an area, such as the area of the face, that is within a circle having a diameter of no more than about 16 cm (about 6 in) or any appropriate dimension that may allow ease of movement by a user. Thus the area of the face **601**, which may be equivalent to the area of the coils, may be about 200 cm² or less. The size of the mobile localizer **600** may, however, be selected based upon an ergonomic consideration for ease of use by a user, such as a one handed use by a user. Thus, the area of the face **601** may be less than 200 cm². The mobile localizer **600** may also include a volume that is about 1200 cm³ or less.

Nevertheless, the mobile localizer **600** may be moved such that the field LF is not obstructed or interfered with by an object O. The mobile localizer **600** may be moved by a user in any appropriate direction, such as arrows **600a**, **600b**. It will also be understood that the mobile localizer may be moved to a new location to ensure that no or little obstructions interfere with the field LF. Also, even if the field LF is less than the surgical area SA, the mobile localizer may be moved to ensure that the entire area SA is covered by the field LF at a time. Thus the small mobile localizer **600** and the field LF may be used to cover a large area without requiring a large static or acquired localizer. Nevertheless, both may be used together or separate. For example, the coil array **46** may be used until the object creates interference, then the mobile localizer could be used. Thus the tracking system **44** may switch between the coil array **46** and the mobile localizer **600** or the two may be used together.

Moving the field LF may increase the accuracy or assist in determining the position of the DRF **54** or a coil in a sensor. For example, although the surgical area SA may be an area including one or more of the DRFs the object O may affect the field LF more in a first position than a second position. The mobile localizer **600** may be moved to assist in reducing the effects of the obstruction O. Further, as discussed herein, various techniques may be used to determine a least affected coil or sensor. The mobile localizer **600** may be moved to assist in decreasing the interference and increase the number of accurate coils or sensors.

It will be understood that the mobile localizer may be held by a hand or on a moveable portion for use. For example, the mobile localizer **600** may be clamped or held relative to the bed **56**. Also the mobile localizer may be held by a user not performing the procedure.

The mobile localizer **600** may be positioned relatively close to a selected portion of the patient **14** for determining a location of a portion, such as a DRF **54** or an instrument. For example, the DRF **54** may be positioned relative to the patient **14**, such as subcutaneously using the subcutaneous DRF **560**. The mobile localizer **600** may be positioned at a small distance, such as less than about one meter from the patient **14**, to localize the DRF **54**. It will be understood, however, that the mobile localizer **600** may be positioned at any distance from the patient **14**, such as less than about twenty centimeters or less than about fifty centimeters. Regardless, the mobile localizer **600** may be positioned substantially near the patient **14** for various purposes.

For example, the mobile localizer **600** may be easily or efficiently moved relative to the patient **14** to substantially reduce metal effects on the field produced by the mobile localizer. As discussed above, the mobile localizer **600** may produce an electromagnetic field that is used by the system **44** to determine a location of the DRF **54** relative to the

mobile localizer **600**. Therefore, the navigation system **44** may be used to determine the position of the DRF on the patient or a selected position of the DRF **54** relative to a second DRF **54'**.

Further, the mobile localizer **600** may be used to reduce interference from various portions or materials that may be present near the patient **14**. For example, the operative bed **56**, the imaging device **12**, or other portions in a selected theater, such as an operating theater, may produce interference that may otherwise need to be accounted for in the tracking system **44** to determine an accurate position of the DRF **54**, or other trackable portion. Positioning the mobile localizer **600** substantially near the DRFs **54**, **54'**, however, may be used to substantially remove various interferences that may otherwise need to be accounted for. The removal of interferences may allow for simplifying various portions of the tracking system **44** or eliminating various algorithms that would need to be used to account for the interferences.

The mobile localizer **600** may be used, as discussed above to determine a location of a tracking sensor. The tracking system may determine a position of the sensor, such as one included in a DRF or the instrument **52**, relative to the patient **14** in the image space. As the mobile localizer **600** is moved relative to the patient **14** and the various tracking sensors, the position of each can be determined with reference to the fixed DRF **54**, or DRF **54'**. The position of the DRFs **54**, **54'** may be known or registered to the image space so that they may also be displayed on the display **36**.

Further, the mobile localizer **600** may also be fixed to the patient **14**. The mobile localizer **600**, as fixed to the patient, may then produce the field LF relative to the patient **14** from the fixed point on the patient **14**. In this instance the position of the various tracking sensors may be determined to the fixed position of the mobile localizer **600** on the patient. Thus, it will be understood, that the mobile localizer may be held by a user or fixed directly to the patient **14**.

In either instance, whether held by a user or fixed to the patient **14**, the effect of various interferences may be reduced or eliminated. The field LF may be formed at and directed closer to the surgical area SA or area of interest with a lower instance of interfering objects O. Also, the mobile localizer **600** may be positioned and aimed or directed toward the surgical area SA in a manner to eliminate obstructions O from the field LF.

In addition, the mobile localizer **600** may be easily used to perform localization and verification purposes, such as various optimization or verification steps may occur. For example, the field strength produced by the mobile localizer **600** may be substantially tuned, depending upon the position of the localizer **600** relative to the patient **14** or the DRFs **54**, **54'**. The field strength, or other feature, may be tuned or changed depending upon a selected local environment. The tuning may be used to increase the efficiency of the mobile localizer **600** and increase its accuracy. Regardless, the field strength need not be tuned for the mobile localizer **600** and it may be used to perform the localization according to various methods.

Further, the mobile localizer **600** may be integrated into any appropriate instrument. For example, the mobile localizer may be integrated into various instruments, such as the probe **66** or the stylet **52**. The mobile localizer **600** may be integrated into the instruments to reduce the number of instruments or portions in a selected operating theater and/or for simplifying the performance of selected procedures. Therefore, the mobile localizer **600** may be moved with the various instruments to assure that the localizer is positioned near the DRF or the selected tracking sensor for determining

a position of the tracking sensor. Also, as discussed above, the mobile localizer **600** may be incorporated into an instrument fixed relative to the patient **14**, thus possibly eliminating the DRF.

For example, the mobile localizer **600** may be integrated into the probe **66**, such that the field generated relative to the probe **66** may be substantially tuned to provide a precise location of the probe **66** for the navigation system **44**. As discussed above, the field strength may be substantially tuned for various applications to achieve selected results. In addition, providing the mobile localizer **600** near to a selected sensor, as discussed above, may substantially reduce metal interference and improve metal immunity.

Therefore, it will be understood, that the mobile localizer **600** may be used to increase efficacy of the tracking system **44** according to various embodiments. Although the mobile localizer **600** may not be required in various applications, the mobile localizer **600** may be used to improve metal immunity and reduce interference that may otherwise need to be accounted for. Further, the mobile localizer may be positioned in various orientations relative to the patient **14** or the localizer sensors, such as the DRFs **54**, **54'** for achieving a more precise signal.

Various systems, algorithms, and the like may be provided to further assist in increasing accuracy and efficacy of the navigation system **44**. For example, a plurality of coils, such as greater than about two coils for an electromagnetic system, may be positioned in a sensor, such as a DRF. For example, any appropriate number of coils may be positioned in a DRF to be localized with the coil array **46** or the mobile localizer **600**. The various coils may be used to provide an accurate determined position of the sensor, according to various embodiments. For example, various averaging methods, weighting methods, or selection methods may be used to determine a most precise sensed or determined location.

Various methods, according to various embodiments, may be used to determine a location of a sensor, such as the DRFs **54**, the probe **44**, the instrument **52**, or any other appropriate portion. As discussed above, the various elements may include electromagnetic portions or coils that allow for sensing and determining a location of the sensor. The determined position of the sensor can assist in determining or interpreting a location of a portion attached to the sensor, such as the instrument, a portion of the patient, and the like. For example, each of the electromagnetic sensors may include one or more of conductors or inductive coils in which a magnetic field may be induced or sensed. As one generally skilled in the art will understand, a magnetic field may be produced with various elements, or a field or current may be induced in the sensor. Therefore, it will be understood that any appropriate portion may be used to form an electromagnetic field or induce an electromagnetic field in the sensor for various purposes.

Further, one skilled in the art will understand that a magnetic field produced or induced in a selected portion may include both a determinable position and orientation. Therefore, these sensed or determined positions and orientations may be used to determine a position of a sensor, such as the DRF **54**. Nevertheless, for various reasons, a plurality of sensors or coils may be positioned in a sensor, such as the DRF **54**. For example, various redundancies and increased accuracy may be achieved by providing a plurality of coils or sets of coils within the DRF **54**, or any appropriate portion, for determining a location and orientation of the DRF **54**. It will be understood that the discussion herein, though directed to the DRF **54**, may be used in any appro-

appropriate sensor for various portions, such as the instrument **52**, the probe **44**, or any other portion. The DRF in the discussion of the following methods and apparatuses is merely exemplary.

With reference to FIG. **31**, a selected algorithm or method of averaging signals **620** is illustrated. The averaging method **620** may generally allow for averaging a plurality of sensed positions or points, such as a position and orientation of a magnetic field, for determining a location of the DRF **54**. Generally, the averaging method **620** may make use of a plurality of sensed locations and averaging methods to provide a precise position of the sensor including the plurality of coils.

The averaging method **620** generally starts at start block **622**. In the start block **622**, the DRF **54** may be positioned on the patient **14** (with reference to FIG. **1**) or any other appropriate location. It will also be understood that various other steps may occur, such as registering the position of the DRF **54** relative to the patient **14** and image space, if so required. It will be further understood that the navigation system **10** may include the monitor **34** that may provide an image **36** of image space of the patient **14** and the position of the DRF **54** relative to the image space may be used. As discussed above, the DRF **54** may be used to insure that the patient space is registered and matched to the image space for performing a selected procedure.

After the procedure is initiated or started in block **622**, magnetic field information may be received from the coils in block **624**. It will be understood that the magnetic information collected from the various coils may include the position and orientation of the magnetic fields produced or induced in the coils or any other appropriate information. Further, it will be understood that the DRF **54** may include any appropriate number of coils, such as one, two, three, four or any appropriate number. Further, any appropriate number of sets of coils may be provided. For example, two sets of two coils may be provided in the DRF **54** at a known or selected geometry for various purposes, such as those discussed herein. Nevertheless, each of the coils may be allowed to produce magnetic field information that may be collected in block **624**. Also, more than one of the DRFs **54** may be used together, such as discussed above. The localizer or tracking array may be used with any appropriate number of the DRFs.

Briefly, as discussed above the sensor or DRF **90** may include the first coil **96** and the second coil **98** (FIG. **6**). As illustrated the coils **96**, **98** may be placed in a selected geometry, such as an angle, relative to one another, such as an orthogonal angle. Although both coils **96**, **98** may be formed about a single axis or origin. It will be understood that any appropriate number of coils may be formed in the DRF **90**, or any appropriate DRF. Thus three or more coils may also be formed generally orthogonal to one another about the single axis.

In addition to the DRF, such as the DRF **90**, including more than one coil, the DRF could include a plurality of sets of coils. With reference to FIG. **27** the DRF **560** may include the first coil sensor set **564a**, the second coil sensor set **564b**, and the third coil sensor set **564c**. Though any appropriate number of sensor coil sets may be provided, three are exemplary illustrated. The coil sets **564a**, **564b**, **564c** may be arranged in the DRF **560** in a selected geometry, such as shape, orientation, separating distance and the like. The geometry of the coil sets **564a**, **564b**, **564c**, may be known and used in various techniques to determine the position of the DRF **560**. It will be understood that any appropriate

sensor, DRF, or member may include the coil sets, coils, and the like to assist in determining a position of the member.

The magnetic field information collected in block 624 of the coils and/or sets of coils may be transferred to the work station 48 or any appropriate processor, such as a microprocessor. As discussed above, the information may be transferred through various wired portions or may be transferred substantially wirelessly. Therefore, it will be understood that the DRF 54 using the method 620 may be a substantially wireless or wired instrument.

The positions of the coils may be computed in block 626 according to various methods, such as those described above or described in U.S. Pat. No. 5,913,820, entitled "Position Location System," issued Jun. 22, 1999 and U.S. Pat. No. 5,592,939, entitled "Method and System for Navigating a Catheter Probe," issued Jan. 14, 1997, each of which are hereby incorporated by reference. It will be understood that any appropriate methods may be used to compute the positions of the received coils or the magnetic field information received from the coils. Further, as discussed above, the position of various portions, such as the patient 14 in the image space or of the instrument 52 relative to the DRF 54 may be also determined. Therefore, the computation of the position of the coils in block 626 may be any appropriate computation and further may include various other relational computations.

After the position of the coils is computed in block 626, an averaging or combination technique in block 628 may be used to average the computed position. In block 628, the various computed positions of the coils from block 626 may be geometrically combined using various methods. For example, a Single Value Decomposition (SVD), as is known in the art, may be used to average the various computed positions of the coils in block 626. Further, it will be understood that other averaging methods may be used to average the computed positions of the coils from block 626. For example, averaging the positions, using other known least squares fit computation or any other appropriate averaging method may be used. Regardless, the various or plurality of computed positions of the coils from block 626 may be averaged or combined in block 628.

The combined or averaged positions in block 628 may be used to determine a final position of the DRF 54. The various positions computed in block 626 may each be a coil positioned within the DRF 52. Therefore, each of the coils may provide a position of the DRF 54. Nevertheless, to assist in assuring accuracy or reduce the effects of interference, such as metal, space, etc., the plurality of coils, for which positions are determined or computed in block 626, may be averaged in block 628 to possibly increase the accuracy of determining the position of the DRF 54. In other words, only a number of the coils, generally less than all of the coils or coil sets would be affected by interference, or the signals received by them. Thus averaging the interfered and non-interfered coil signals reduces, to an acceptable level, or eliminates error that may be created by the interference.

Further, in block 628 the various degrees of freedom, such as a six degree of freedom (6 DOF) transform may be determined. Thus, the combination of the various computed positions of block 628 may provide information regarding the position and orientation of the DRF 54 in a substantially precise manner. As discussed above, averaging the position of the plurality of coils in block 628 may provide for a plurality of position information for the DRF 54.

Finally, the navigated position may be displayed in block 630. The position of the DRF 54, the instrument 52, or any appropriate portion may be displayed on the monitor 34. As

discussed above, the image space may be registered to the patient space or a position of the instrument may be displayed on the image space relative to the patient 14. Therefore, the navigated position determined using the method 620 may be displayed in any appropriate manner. As discussed above, the display may include the monitor 34, may be a heads up display for the physician 614, or any appropriate display.

With reference to FIG. 32, a selection method for determining a position of the DRF 54 is illustrated. It will be understood that although the selection method 640 may be discussed in relation to the DRF 54 that the selection method 640 may be applied to any appropriate portion. For example, the selection method 640 may be applied to determining and displaying a position of the instrument 52, the probe 44, or any appropriate portion. Therefore, the discussion herein related to the DRF 54 is understood to not be limited to the DRF 54 alone.

The selection method 640 generally starts in block 642. As discussed above, various procedures may occur prior to the start block 642. For example, registering the image space to the patient space may be performed or positioning of the DRF 54 on the patient 14 may be performed. Further, various images may be obtained preoperatively of the patient 14 for use in the selection method 640. Regardless, the selection method may generally begin at block 642 and allow for determination of the position of the DRF 54.

Similar to the averaging method 620, information regarding the magnetic field may be collected in block 644. Further, the position of the each of the coils may be computed in block 646. As discussed above, each of the DRFs 54 may include a plurality of coils, such as any appropriate number for use in the method 640. Each of the plurality of the coils may include unique magnetic field information, such as orientation and position. Further, a plurality of sets of the coils may be provided in the DRF 54, such as those described above in relation to FIGS. 6 and 27. Each of the coils and/or each of the sets of coils may be positioned at a known or selected orientations or geometry relative to one another. The known respective or relative positions or geometry may be generally fixed relative to each of the coils or sets of coils for use in the selection method 640.

Once the position of the each of the coils or sets of coils is computed in block 646, the six degrees of freedom transform may be computed in block 648. It will be understood that the 6 DOF transform may be computed for each of the coils or the coil combinations according to various generally known methods, such as those described above or in U.S. Pat. No. 5,913,820, entitled "Position Location System," issued Jun. 22, 1999 and U.S. Pat. No. 5,592,939, entitled "Method and System for Navigating a Catheter Probe," issued Jan. 14, 1997, each of which are hereby incorporated by reference. The 6 DOF transform may be computed to determine the geometry or position of the coils or sets of coils relative to one another.

In block 650, the computed geometry of the coils in block 648 may be compared to a known geometry in block 650. As discussed above, the coils or sets of coils may be positioned in the DRF 54 or any appropriate portion at generally known or specifically known geometry. The computed geometry in block 648 may therefore be compared relative to the known geometry in block 650.

For example, three coil sets may be positioned in the DRF 54. Each of the coil sets may include or be computed to have a sensed geometry or position in block 646 and 648. The computed positions of the three coil sets may then be

compared to the known positions of the three coil sets in block 650. For example, if the first coil set is known to be at a known position relative to the second and third coil set, while the second coil set is known to be at a selected and known position, relative to the first and third coil sets, and finally the third coil set is at a selected and known position relative to the first and second known coil sets, those known positions may be compared to the determined or calculated positions in block 648. Therefore, each of the coil sets may be compared to the known positions of the coil set to the other coil sets. This comparison may be used to determine which coil set is least affected by various interferences.

The coil sets or coils least affected by interferences may be used to determine the position of the DRF 54. As is known various items may interfere with a magnetic field produced or induced in the coils. Nevertheless, a position of the coils may be sensed and a sensed geometry may be compared to the known and/or saved geometry of the coils. As discussed above, the coils are generally fixed relative to one another. Therefore, in block 654 the coil set that gives the closest match to the known geometry may be selected. The coil set that most closely matches the known geometry is most likely the coil set least affected by interferences. The coil set least affected by interferences may provide the most accurate position of the DRF 54 for determining a location of the DRF 54 relative to the patient 14 and for determining a position of the patient relative to the image space.

Once the coil set is selected that is closest to the known geometry, a position of the DRF 54 or the instrument 52, or any appropriate portion may be displayed on block 656. The position displayed on block 656 may be the position of one or more of the coil sets. As discussed above, the plurality of coil sets included for the selection method 640 may be used to select a single coil set to determine a position of the DRF 54. Therefore, only one or more of the coil sets may be used to determine the position and display the navigated position in block 656.

It will be understood that the selection method 640 may be combined with the averaging method 620 to determine or display a position of the DRF 54. For example, a plurality of coil sets such as the three, may be included for the selection method 640. More than one coil set may be selected in block 654 as being close or equally close to the known geometry. Therefore, the averaging method 620 may be used to average the two or more selected coil sets to provide further refinement for determining a position of the DRF 54. Therefore, after block 654, selecting the coil sets closest to the known geometry, the method may proceed to block 628 of the averaging method 620 or may proceed directly to block 656. That is the selected coil sets may be geometrically combined or averaged in block 628. After combining or averaging the coil set in block 628, the position of the DRF may then be displayed in block 656. Therefore, it will be understood, that any method may be used in combination with any other method or methods to determine a position of the DRF 54.

With reference to FIG. 33, various methods may be used to determine a position of the DRF 54. For example, a weighting method 660 may be used to determine a position of the DRF 54. It will be understood, as discussed above, that a position of the DRF 54 is merely exemplary and not limited. Therefore, the weighting method 660 may be used to determine the position of the instrument 52, the probe 44, or any appropriate portion, such as an implant, to the patient 14 for displaying the image space 36. Therefore, the discussion below related to the DRF 54 is intended to be exemplary and not limiting.

The weighting method 660 may generally begin at block 662. As discussed above, the start block 662 may include any appropriate preparation or steps, such as positioning the DRF 54, obtaining images of the patient 14 or any appropriate steps. Merely starting at block 652 is exemplary and it will be understood to include any appropriate portions.

Further, as discussed above, magnetic field information may be collected from the various coils in block 664. The collection of magnetic field information may be collected from any appropriate number of coils, such as two coils, three coils, or any appropriate number of coils. Further, various magnetic field information may be collected from the sets of coils, rather than individual coils.

Magnetic field information collected from the coils may also include information other than position and orientation of the field. For example, as one will understand, various other information, such as phase angle, frequency response, and other information regarding the navigation of the instrument or the DRF 54 or information collected from the sensors in the DRF 54 may be collected in block 660. These various pieces of information may be collected when the field information regarding the coils is collected or at any appropriate time.

The various data or information collected in block 664 may be used to weight the information collected in block 666. Weighting the information in block 666 may be used to determine or assist in determining the integrity of the information collected in block 664. Various portions or materials, such as metal immunity, and the like, as discussed above, may affect the information collected in block 664. The various materials may also affect the additional information. Thus the various additional data may be used to determine a relative effect of the various portions on the field information being collected in block 664.

The additional information that may be collected in block 664, besides position and orientation of the magnetic field, may be used to weight the information collected in block 664 to assist in determining the position of the various coils and the DRF 54. The weights may be applied in block 668 to the various pieces of data or to the equations regarding determining or evaluating the positions of the coils or the DRF 54. Once the weights are applied in block 668, the 6 DOF or position and orientation of the coils or the DRF 54 may be computed in block 670. For example, coils or coil sets that appear or are being affected more by interference may be weighted less than those that are less affected. Thus, all information may be used according to its known or determined weight, which can increase the accuracy of the tracking system.

Various methods may be used to compute the position or geometry of the coil or coil sets, such as those discussed above, or generally known in the art. Various methods may be used to compute the position of the coils where the DRF 54 using the weighted data to determine a position in orientation of the DRF 54 relative to the patient 14 and for navigation.

Once the position and orientation is computed in block 670 with the weighted data or equations, the navigated position may be displayed in block 672. As discussed above, the navigated position may be displayed at any appropriate display for various applications.

Therefore, it will be understood that according to various embodiments, more than one coil may be used to determine a position of an instrument, such as the instrument 52, the DRF 54, an implant (such as those discussed above), the probe 56 or any appropriate portion. The positions of the coils may be used to register the image space to the patient

space, real-time register the image space to the patient space, or determine a position of the instrument, relative to the patient 14. Regardless, the plurality of methods, or any appropriate method, may be used to collect data from a plurality of coils. As discussed above the plurality of coils may be positioned in a single portion, such as a single DRF, a single instrument, or the like, to assist in precisely determining the position of the instrument, the DRF, or the like. Thus, any appropriate portion or method may be used to assist or determine a position of the DRF.

According to various embodiments, including those discussed above, various methods may be used to determine a position or axis of a portion of the patient 14. Various anatomical landmarks or geometries, such as an axis of a femur, humerus, or the like may be determined. For example, a transepicondylar axis may be determined by determining or finding a position of a first epicondyle, such as a medial epicondyle, and a second epicondyle, such as a lateral epicondyle.

With reference to FIGS. 34A and 34B, a distal end of a femur 700 may be provided as a portion of the patient 14. It will be understood that the femur 700 is generally surrounded by a portion of soft tissue 702, including skin, fascia, muscle, and the like. It will be understood that the FIGS. 34A and 34B are diagrammatic for ease of the following discussion and are not detailed for clarity. The distal end of the femur 700 may include a plurality of landmarks, including a first epicondyle 704, and a second epicondyle 706. It will be understood that the epicondyles 704, 706 may be any appropriate epicondyle of the femur 700. For example, the femur 700 may be a left or right femur and thus the epicondyle 704, 706 may be medial or lateral condyles, depending upon the femur selected.

Regardless, the epicondyles 704, 706 may define a transepicondylar axis 708. The transepicondylar axis 708 is generally an axis or a line between the epicondyles 704, 706 drawn across or through the femur 700.

The transepicondylar axis 708 may be used for any appropriate procedure, such as a total knee arthroplasty (TKA). The transepicondylar axis 708 may be used for positioning an implant, forming a resection of a distal portion of the femur 700, or any appropriate reason. Nevertheless, determining the transepicondylar axis 708 may be performed using an ultrasound probe 710 and generally associated ultrasound equipment.

The ultrasound probe 710 may produce a cloud of points or information, such as the area 712 relative to the epicondyle 706 or area 714 relative to the epicondyle 704. As discussed herein, this mosaic method may be used to determine a selected point. The ultrasound may be any appropriate ultrasound, such as a mode A or a mode B. Regardless, the ultrasound probe 710 may be moved across the soft tissue 702 relative to the femur 700 for determining the epicondyle 704, 706. Various systems for using ultrasound systems for registration are disclosed in U.S. Pat. Nos. 6,106,464 and 5,398,875. It will be understood that the ultrasound probe 710 may also include a tracking sensor, similar to the DRF sensor, to allow the tracking system to track the position of the ultrasound probe relative to the patient for use in the tracking system 44. The various images and displayed images of the position of the ultrasound probe 710 may be displayed on the display 34.

As is understood by one skilled in the art, the ultrasound may produce ultrasonic waves that may be used to determine a position of a selected anatomical portion through the soft tissue 702. Therefore, the ultrasound probe 710 may be used to determine various anatomical points, such as the epicon-

dyle 704, 706 without invading or passing through the soft tissue 702. In addition, the ultrasound probe 710 may be used to determine various anatomical landmarks or points using a substantially minimally or less invasive procedure when exposing the entire or distal end of the femur 700 is not generally performed.

As discussed above, the area of information 712, 714 generally near the epicondyle 704, 706 may be used to determine or compute the position of the epicondyle 704, 706. For example, the most medial or lateral points in the information areas 712, 714 may be used to determine the position of the epicondyles 704, 706. These points may be determined to be "high" points in the areas 712, 714 and may be determined to be the epicondyles 704, 706 of the femur 700. It will be understood that various methods may be used to determine the positions of the epicondyle 704, 706 according to various embodiments.

The determined points of the epicondyle 704, 706 may be displayed relative to a patient image, such as a pre-acquired or preoperative CT scan, MRI scan, x-ray, or the like. Therefore, the determined epicondyle axis 708 may be displayed on a display or image space of the patient 14 without piercing the soft tissue to expose the femur 700. This may allow for intra-operative planning and determining of the procedure without producing further incision in the patient 14.

Further, the ultrasound probe 710 may be used to determine various other anatomical axes or points. For example, a posterior condylar axis, anterior cortex point, tibial tubercle, anterior-posterior femoral axis, and the like may be determined with the ultrasound probe 710 and various navigation displays. For example, the navigation system 10 may be used with the ultrasound probe 710 to assist in displaying on the display 34 an image of the patient 14 and the determined transepicondylar axis 708. Therefore, the display 34 may display a non-invasively determined anatomical axis for use by a user, such as a physician for planning or performing a selected procedure.

With reference to FIG. 35, the patient 14 may include a bone, such as a femur 800 relative to a tibia 802. The bones, such as the femur 800 and the tibia 802, may be surrounded by various portions of soft tissue 804, including skin, muscle, etc. The bones, such as the femur 800 are generally substantially contiguous and integral but may become damaged due to disease, injury, or the like. For example, a fracture 806 may form in the femur 800. The fracture 806 may be repaired or held together such that the femur 800 may again act as an integral bone with the various portions. For example, an intramedullary (IM) rod 808 may be provided through an intramedullary canal of the femur 800. The IM rod 808 may span the fracture 806 such that two or more portions of the femur 800, or any appropriate bone portion, may be held relative to one another for use. The IM rod 808 may be positioned to allow for healing of the fracture 806 or for permanently holding the portions of the femur 800 relative to one another. It will be understood, that although the following discussion relates generally to the IM rod 808 and its use in a femur 800, that any appropriate bone portion or implant may be used to achieve a similar result.

Regardless, the IM rod 808 may be positioned through the intramedullary canal of the femur 800 to span the fracture 806. It may be desired, however, to further fix the IM rod 808 relative to the femur 800 to ensure that the various portions on the other side of the fracture 806 are held relative to each other. Therefore, a fixation screw or pin 810 may be provided that is operable to pass through a portion of the femur 800 and a portion of the IM rod 808, such as a bore

812 formed in the IM rod **808**. It will be understood that a plurality of screws may be used to fix the IM rod **808** relative to the femur **800** in a plurality of positions or a plurality of points. Regardless, the screw **810** is generally positioned such that it is operable to pass transversely through the bore **812** and not another portion of the IM rod **808**.

The IM rod **808** may further include one or more of a tracking sensor **816**. The IM tracking sensor **816** may be used to track a position of the IM rod **808** with the tracking system **10**, according to various embodiments. Further, the tracking sensor **816** may be any appropriate tracking sensor, such as those described above. Nevertheless, the tracking sensor **816** may include an electromagnetic tracking sensor, an acoustic tracking sensor, a radiation tracking sensor, an optical tracking sensor, or any appropriate tracking sensor. The tracking sensor **816** may be tracked using the array **46** or the mobile localizer **600** according to various embodiments. This may allow for determining a position of the IM rod **808** and a bore **812** in the IM rod **808**. The IM rod **808** may be used in an image or imageless system for tracking the position of the IM rod **808**. Regardless, the position of the IM rod **808** is tracked relative to the screw **810**, or vice versa.

The screw **810** may also include a tracking sensor **820** that is operable to be tracked with the tracking system similar to tracking the tracking sensor **816** in the IM rod **808**. Therefore, the screw **810** may be tracked relative to the bore **812** in the IM rod **808**. The tracking system may then be used to determine whether the screw **810** is positioned or will be inserted on a selected path to allow it to intersect to the bore **812** after insertion into the bone **800**.

The bone **800** may also include a DRF thereon, which may be any appropriate DRF, such as those described above. Therefore, the image space of the system may be registered relative to the patient space and the DRF **54** is used to maintain the registration should movement of the femur occur. Further, the IM tracking sensor **810** may be used to track a position of the IM rod **808** and the bore **812** in the IM rod **808** relative to the screw **810**. This may allow the screw **810** to be passed along a selected path, such as a path **824**, to ensure that the screw **810** engages and will pass through the bore **812** in the IM rod **808**. Thus, the tracking sensors **816**, **820** may be used by the tracking system in lieu of other instrumentation to ensure proper alignment of the screw **810** relative to the bore **812**.

Further, it will be understood that any appropriate implant may be positioned relative to the anatomy. For example, rather than providing the IM rod **808**, the implant may be a bone plate **830** implant that is operable to span the fracture **806**.

With continued reference to FIG. **35**, the bone plate **830** may also be provided, or as an alternative to the IM rod **808**, to span the fracture **806**. The bone plate may also include a bore **832** through which the screw **810** or any appropriate screw may pass. In addition, the bone plate **830** may include a tracking sensor **834** such that a position of the bone plate **830** may be tracked. Therefore, as with the IM rod **808**, the screw **810** may be tracked relative to the bone plate **830** such that the screw will pass through the bore **832** to allow for fixation of the bone plate **830** relative to the bone **800** with the screw **810**.

The various tracking sensors **816**, **820**, **832** may be used to allow for alignment of the screw **810** relative to the selected portion through a substantially small or minor incision **840**. In this way the incision may remain small, but the positioning of the incision and the screw **810** relative to the portion through which the screw will pass may be

substantially precisely determined, planned, and tracked with the tracking system. Therefore, a substantially open procedure or one requiring various other external mechanisms, such as alignment guides generally known in the art, may be reduced by using the tracking system. The tracking system is operable to allow for precise alignment of the screw **810** relative to the portion through which it must pass to allow for proper positioning of the implant relative to the bone **800** may be maintained.

Further, the various tracking sensors may be any appropriate tracking sensors. For example, the tracking sensor may be integrated into the implant such as the IM rod **800**, the screw **810** or the bone plate **830**. However, the tracking sensor may also be rigidly attached with selected portion, such as the implant or an instrument positioning or holding the implant relative to the anatomy. Various connectable or engageable tracking sensors include those disclosed in U.S. Pat. No. 6,499,488 issued Dec. 31, 2002 entitled "Surgical Sensors", incorporated herein by reference. Therefore, it will be understood that the tracking sensor may be any appropriate tracking sensor and may be either integrated into the implant or instrument or selectively attachable thereto.

Further, the DRF **54** or any appropriate tracking sensor positioned relative to the femur **800** or the tibia **802** may be used by the tracking system to determine motion of the bones relative to one another. The motion or articulation of the bones, such as the femur **800** relative to the tibia **802**, may be used to determine an anatomical plan, a range of motion, a joint line, a distance between various bones, or any other appropriate measurement. The tracking sensors may be tracked by the system to display motion of the various portions of the anatomy on a display or for determining measurements of the anatomy. For example, this may be used to determine a position of the implant, such as the IM rod **808** or the bone plate **830** relative to the bone or any appropriate implant, such as an articulated implant or the like.

The various portions of the anatomy may be measured to ensure that an appropriate distance, pre- and post-operatively is achieved or any other appropriate measurement. For example, when repairing the fracture **806**, a length of the femur **800** may be selected. Various tracking sensors, including the DRF **54**, may be used to assure that the selected length is achieved post-operatively or intra-operatively, or if further adjustment is necessary. Various types of joint measurements are disclosed in U.S. Pat. No. 5,772,594 to Barrick, issued Jun. 30, 1998, incorporated herein by reference. Regardless, the tracking sensors used may include the tracking sensors discussed above and may be used by the tracking system to ensure or assist in planning or determining the achievement of a selected surgical plan.

Various instruments can be used to perform the various procedures, such as positioning implants, performing resections, positioning implants, and the like. The various instruments can be tracked to display a position of the instrument during the operative procedure. The tracking can be done with tracking sensors that can be positioned near or at a distal or working end of the instrument, or at any appropriate position on the instrument.

As discussed above, various instruments can be used during a surgical procedure. For example, an instrument **900** can be an awl, probe, tap (APT) instrument, as illustrated in FIG. **36**, according to various embodiments. The instrument **900** can include a general or universal tool portion **902** and an interchangeable portion **904**. The interchangeable portion **904** can be any appropriate portion such as a screw tap, a probe, or an awl. It will be understood that the interchange-

61

able portion **904** can also be any other appropriate member, such as a screw, a nail, a fixation pin or the like. The interchangeable member **904** can be any appropriate member that is operable to interchange with the standard portion **902** in an operable manner. The interchangeable member **904** may include a quick connect portion, a tool engagement portion, and a thread portion, or the like, to connect with the tool portion **902**.

The tool portion **902** and the interchangeable portion **904** can be formed of any appropriate materials. As discussed herein, the instrument **900** can be tracked using an electromagnetic tracking system or any other appropriate tracking system. If an electromagnetic tracking system is used, it may be selected to form the instrument **900** of a non-ferrous material such that it is not likely to interfere with the electromagnetic tracking system. Therefore, the instrument **900** can be formed of titanium, other non-magnetic alloys, non-magnetic synthetic materials, or any appropriate materials. It will be understood that the various instruments described herein that are used with the electromagnetic tracking system may all be formed of non-magnetic materials or any other appropriate materials.

The instrument **900** can be used with the navigation system **10**. The navigation system **10** can be an image or an imageless navigation system. That is, as discussed above, images can be acquired of the patient **14** and displayed on the display **34**. Further representations of various instruments, such as the instrument **900**, can also be displayed on the display **34**. Alternatively, the navigation system **10** can be substantially imageless such that the instrument **900** is illustrated relative to a selected point.

The navigation system **10** can be any appropriate navigation system, such as an electromagnetic navigation system as discussed above. The instrument **900**, therefore, can include a tracking sensor **906**. The tracking sensor **906** can be positioned at any appropriate position relative to the instrument **900**. The tracking sensor **906** can generally be interconnected with a bobbin or interchangeable member **908**. The interchangeable member **908** can include a tool engaging end **910** that can include a quick connect portion that can interconnect with a tool engaging shaft **912**. The interconnecting portion **908** can further include a handle engaging end **914** that is operable to engage a handle **916**. The connections can be any appropriate connections such as quick connections, permanent connections, threaded connections, or the like.

The tracking sensor **906** can be positioned at any appropriate position, but can be interconnected with the interchangeable member **908** such that the tracking sensor **906** is present in the various handles **916** and shafts **912** can be interconnected with the interconnecting member **908**. The tracking sensor **906** can be positioned at a distance **918** from an axis **920** of the instrument **900**. The distance **918** can be any appropriate distance. For example, the distance **918** can be selected for operation by a user to minimize interference of the tracking sensor **906** with use of the instrument **900**. Nevertheless, the distance **918** can be known and unchangeable so that the position of the tracking sensor **906** relative to the other parts of the instrument **900** can be known for determining a location of any portion of the instrument **900**.

The tracking sensor **906** can be any appropriate sensor or transmitter, such as an electromagnetic sensor including those described above. It will be understood that the tracking sensor **906** can include a plurality of coils, such as three coils, that can be positioned relative to one another in a substantially selected manner. Further, the tracking sensor **906** can be any appropriate EM sensor, such as a Hall Effect

62

sensor. Thus, the use of coils is not required, but is merely exemplary. For example, the three coils can be positioned substantially orthogonal to one another and in a substantially fixed orientation to allow for up to six degrees of freedom of tracking. The various types of the tracking sensors can include those described above or any appropriate tracking sensor.

The tracking sensor **906** can be wired or hard wired to the tracking system that is interconnected with a connector **920** and a wire **922**. It will be understood that the tracking sensor **906** can also be a wireless sensor. The connector **920** can be interconnected with the navigation probe interface **50**, the isolator circuit **55**, or any combination thereof. It will be understood that the instrument **900** can be interconnected in a manner substantially similar to the probe **52** discussed above. Therefore, the tracking sensor **906** can be used to track the instrument **900** in any appropriate manner. Further, the connector **920** can be any appropriate connector for connection with the navigation system **10**. The illustrated connector **920** is merely exemplary of any appropriate connector.

As discussed above, the instrument **900**, including the distance **918**, the connector portion **908**, the shaft **912**, and the interchangeable member **904** can have positions and orientations substantially known relative to one another. Therefore, the position of the tracking sensor **906** can be known substantially relative to any other portion that is interconnected or interacting with the tracking sensor **906**. Thus, the instrument **900** can be tracked, including any portion, thereof by determining the position of the tracking sensor **906** and calculating a position of any of the other portions of the instrument **900** relative to the tracking sensor **906**.

The instrument **900** can be used for any appropriate procedure. For example, the interchangeable member **904** can include an awl for creating a pilot bore or divot at a location, such as in a spinal portion. A tap can be interconnected as the interconnectable member **904** to form a tapped bore for receipt of a selected screw member. All of these may be used for performing a spinal procedure, such as for fixing a spinal implant relative to a spine or any other appropriate procedure.

With reference to FIGS. **37** and **38**, an instrument **940** is illustrated that can be similar to the instrument **900**. The instrument **940** can include a generally fixed or handled portion **942** and an interchangeable portion **944**. The interchangeable portion **944** can be similar to the interchangeable portion **904** of the instrument **900**. The handle portion **942** can be similar to the handle portion **902** of the instrument **900**. The instrument **940**, however, can selectively not include the interchangeable portion **908**, but simply include the rod engaging or tool engaging portion **946** and an operable handle **948**.

Defined through the instrument **940** is a cannula **950**. The cannula **950** can extend through the handle **948**, the shaft **946** and the interchangeable portion **944**. The cannula **950** can be formed in any appropriate dimension and for any selected instrument, such as those described herein. The cannula **950** can be operable to interact with the stylet **150**. The stylet **150**, including the tracking sensor **162**, as described above according to various embodiments, can be positioned through or in the cannula **950** defined by the instrument **940**. The stylet **150** can include the portions described above and illustrated in FIGS. **10A** and **10B**. Generally, however, the stylet **150** can be positioned in the cannula **950**. As discussed above, the tracking sensor **162** defined by a portion of the stylet **150** can be used to track a

portion of the instrument **940**. As discussed above, positioning the stylet **150** within the cannula **950**, as illustrated in FIG. **38**, can allow for tracking any appropriate portion of the instrument **940** by tracking a position of the tracking sensor **162** defined by the stylet **150**.

It will be understood that the tracking sensor **162** defined by the stylet **150** can be positioned at any appropriate position within the instrument **940**. That is the tracking sensor **162** can be positioned substantially near the interconnectable member **944**, within the interconnectable member **944**, or within the fixed portion **942**. If the tracking sensor **162** is positioned substantially near a distal end of the instrument **940**, such as in the interconnectable member **944** or near the interconnectable member **944**, the tracking sensor **162** can be tracked to determine a substantially precise location of the interconnectable member **944** or the distal end of the instrument **940**.

The stylet **150** can be interconnected with the handle **948**, the shaft **946**, or any appropriate portion of the instrument **940**. Nevertheless, the stylet **150** can be provided in any appropriate dimension such that it is nonbinding inside of the cannula **950**. Therefore, the instrument **940** can move, or at least portions thereof can move, relative to the stylet **150**, in particular the tracking sensor **162**. Therefore, as the interchangeable member **944** is moved relative to a selected portion of the patient **14** it can be deformed or deflected, but its position can be substantially known due to the positioning of the tracking sensor **162** on the stylet **150**.

As discussed above, the interconnectable member **944** can be an awl. Therefore, as the awl is being used a tip of it may deform or deflect, but the position of the interconnectable portion **944** is substantially known. Similarly, if the tracking sensor **162** is positioned substantially near the interchangeable member **944**, the shaft portion **946**, which can be any appropriate length and formed of any appropriate material, can also change its dimensions while the position of the interchangeable member **944** is still known. For example, the shaft **946** can be formed of a deformable material that allows it to flex under a selected load. Although the shaft **946** can flex under a selected load, the positioning of the tracking sensor **162** near or in the interchangeable member **944** can allow for tracking the position of the interchangeable member **944** due to the fact that the tracking sensor **162** formed on the stylet **150** is near the distal end of the instrument **940**.

It will be understood that the tracking sensor, such as the tracking sensor **162**, can be formed in any appropriate manner, for example, the tracking sensor **162** can be formed on the stylet **150** according to any appropriate method such as those described above according to various embodiments. Therefore, the stylet **150** can be formed of any appropriate materials. Nevertheless, it will be understood, that the tracking sensor **162** can be formed on the shaft **946** or on the interchangeable member **944**, itself. Although the selection of the material for the various portions can be chosen to allow for formation of the tracking sensor on the instrument **940** itself rather than the stylet **150**, it will be understood that the stylet **150** can be used interchangeability.

Further, the stylet **150** can be used with any non-unique instrument **940**. That is the stylet **150** can be positioned in any cannulated instrument to allow for tracking of a selected portion of the cannulated instrument. Therefore, the tracking sensor **162** is substantially portable and can be used with any appropriate instrument, such as those already existing in the operating theater. But the stylet **150** still allows for tracking a portion of any appropriate instrument at a working or distal end thereof.

The stylet **150** can be wired including the wire **152**, such as that illustrated in FIG. **10A**. Alternatively, the stylet **150** may include substantially wireless sensors, thus as generally known in the art including those disclosed in U.S. Pat. No. 6,474,341 to Hunter et al., issued Nov. 5, 2002, incorporated herein by reference. Therefore, it will be understood that the tracking sensors **162** can be any appropriate tracking sensors. The stylet **150** can be interconnected with the navigation probe interface **50**, the isolator circuit **55**, or any appropriate portion of the navigation system **10**. Therefore, the stylet **150** can be used to track the position of the instrument **940** or a selected portion of the instrument **940** even though the instrument **940** may become deformed during an operative procedure. In addition, the instrument **940** can be formed of any appropriate materials, including those that are appropriate for the instrument **900**. For example, it may be selected to the instrument **940** of substantially non-magnetic or non-ferrous materials which may include various metal alloys or synthetic materials.

With reference to FIG. **39**, a guide instrument **980** is illustrated. The guide instrument **980** can include various portions such as an external tube **982**, a handle **984**, and a connection or collar portion **986**. The external tube **982** can be substantially hollow and define a cannula and can also include a working end **988**. The working end can allow for operation of any appropriate portion, such as a drill bit relative to the working end **988**. The working end **988** may be interconnected or formed as one-piece with the tube **982** or formed substantially as a single member therewith.

The collar **986** can further define a cannula bore that interconnects with the cannula bore defined by the tube **982**. Positionable within the tube **982** can be a spring **990**, a sleeve **992** that can include a tracking sensor **994** or any appropriate number of the tracking sensors **994**. Positionable within the sleeve **992** is a drill bit **996**. The drill bit **996** can include an extended shaft **998** and a drill tip **1000**. The drill tip **1000** can be any appropriate drill tip. Further, the drill bit **996** can include a stop collar or stop member **1002** for interacting with an appropriate portion such as with a proximal end **1004** of the tube **992**. The collar **1004**, or any appropriate portion, can also allow for a fixed connection of the sleeve to the drill bit **996**. It will be understood that the drill bits **996** may also include a tool engaging portion, such as a proximal end of the drill bit **996**. The tool engaging portion can engage any appropriate tool such as a hand crank drill, a power drill motor, or any other appropriate member. Nevertheless, the drill bit **996** can be positioned within the sleeve **992** to be positioned within the tube **982**.

As discussed above, a substantially hollow cannula such as the suction tube **190** illustrated in FIG. **13** can include the tracking sensors **206**, **208**. It will be understood that the tube **992** can be similar to the tube portion of the suction tube **190** illustrated in FIGS. **13** and **14**. Further, the tracking sensor **994** can be substantially similar to the tracking sensors **206**, **208** described and illustrated above. Therefore, detailed description thereof is not necessary herein.

Nevertheless, the tube **992** can be positioned within the exterior tube **982** to offer tracking by the tracking sensor **994** once the tube **992** is positioned within the exterior tube **982**. As discussed above, the tracking sensors, such as the tracking sensor **994** can be tracked with the navigation system **10**. The tracking sensor **994** positioned on the tube **992** is operable with the drill bit **996** and can allow for tracking of a selected portion of the drill bit **996**, such as a portion substantially near the drill tip **1000**. Therefore, it will be understood that the tracking sensor **994** can be positioned on

any appropriate portion of the tube **992** where the tube **992** can be formed relative to the drill bit **996**.

During an operative procedure, the spring **990** may be positioned in the external tube **992** which can be followed with the sleeve **992** and the drill bit **996**. The drill bit **996** can be positioned within the tracking sleeve **992** and the unit can be positioned within the outer tube **992**. It will be understood, however, that the assembly can be interconnected in any appropriate manner.

During operation, the drill tip **1000** can be advanced towards or out of the working end **998**. As the drill at **1000** is operated, the tracking sensor **994** is able to be used to determine a position of a portion of the sleeve **992** substantially near the drill tip **1000**. The spring **990** can also be used to assist in determining a positioning of the drill tip **1000**. The spring **990** compresses a selected distance during operation of the drill bit **996**. The compression of the spring **990** can be used to determine an exact location of the drill bit **1000** even if the tracking sensor **994** is not substantially on or adjacent the drill tip **1000**. Therefore, the instrument **980** can be used to determine a substantially precise location of the drill tip **1000** during an operative procedure even if the drill bit **996** becomes deformed during an operative procedure.

Further, the sleeve **992** allows for free rotation of the drill bit **996** during an operative procedure, while still allowing for the tracking sensor **994** to be positioned substantially near the drill tip **1000**. As discussed above, the tracking sensor **994** can be formed on the tube **992** substantially similar to the tracking sensors **206**, **208** formed on the tube and the suction tube **190**.

The sleeve can be substantially wired or wireless. For example, a connector **1006** can be interconnected with the tracking sensor **994** and further connected with a wire **1008** to be interconnected with the probe interface **50** or the isolator circuit **55**. The tube **998** may include a recess or slot **1010** that is operable to allow for reveal of the sensor connection **1006**. It will be understood, however, that the tracking sensor **994** can be substantially wireless, as is known in the art.

Further, it will be understood that various portions of the instrument **980** can be formed of selected materials, including those discussed above. The instrument **980** can be formed of substantially non-magnetic materials, including non-magnetic alloys, synthetic materials, or the like. Nevertheless, the instrument **980** can be formed of materials to allow for the tracking sensor **994** to operate effectively to allow for determination of the position of the tracking sensor **994** and position of the various portions of the instrument **980** relative thereto.

As discussed above, positioning the tracking sensor substantially near the working end, such as the drill tip **1000**, can allow for a precise determination of a position of the drill tip **1000** even if the drill tip **1000** moves or is deformed relative to the shaft **998** of the drill bit **996**. Therefore, during an operation, such as during a spinal procedure, a cranial or neurological procedure, or the like, the position of the drill tip **1000** can be substantially precisely known due to its proximity to the tracking sensor **994**.

It will be understood that the tracking sensors, such as the tracking sensor **994** on the instrument **980** or the tracking sensors **162** on the stylet **150** can be provided as a plurality for tracking verification. For example, if two or more of the tracking sensors are provided, then the spatial position, including distance and orientation, between the two or many should be substantially constant due to the materials rigidly relative to the tracking sensors. Therefore, the tracked loca-

tion of the two tracking sensors on the same instrument can be used to determine accuracy of the tracked system.

Further, as discussed above, the navigation system **10** using the tracking sensors near a working end or a distal end of the instrument can allow for reduced calibration of the system. For example, the position of the tracking sensor is known to be near the working end of the instrument. Therefore, a calibration of a length of the instrument is not necessary between the working end of the instrument and the tracking sensor. By positioning the tracking sensor substantially near the working end, the tracking sensor is able to very accurately determine that position of the working end of the instrument, such as a drill tip or an awl.

With reference to FIG. **41**, a tracking sensor **1020** is illustrated. The tracking sensor can be any appropriate tracking sensor and may exemplarily be used as a dynamic reference frame, such as the dynamic reference frame **54**. The tracking sensor **1020** can be used as a dynamic reference frame and can include a fixation base **1022** for fixation to a selected anatomical portion, such as a boney portion including a spinal process, a femur or any other appropriate boney portion. The fixation base can include a bone engaging screw portion **1024** and a fixation platform **1026**. The fixation platform can include teeth or projecting members **1028**. The projecting members **1028** can engage the bone to assist in reducing rotation of the base **1026** relative to the portion to which it is fixed. Therefore, rotation of the tracking sensor **1020** can be substantially reduced or eliminated to allow for greater degrees of freedom of tracking.

The tracking sensor **1020** further includes a tracking head **1030**. The tracking head **1030** can include the tracking sensor coils **1032**. The tracking sensor coils **1032** can be any appropriate coils such as the coil **90** illustrated in FIG. **6**, according to various embodiments. Nevertheless, as discussed above, the tracking head **1030** can use any appropriate sensor, rather than only coils. It will be understood that the sensor may be any appropriate sensor, such as any appropriate EM sensor including Hall Effect sensors. Although the tracking coils **1032** can be fitted inside of the cap **1030**, such as through molding or casting, the tracking coils **1032** can be fitted to the cap **1030** according to any appropriate manner.

The cap **1030** further includes a base engaging portion **1034**. The base engaging portion **1034** can engage a portion of the screw **1024** such as a proximal or cap engaging portion **1036**. The interconnection between the cap **1030** and the cap engaging portion **1036** can be substantially firm and resist rotation of the cap, including the tracking coils **1032** relative to the base **1022**, and therefore, relative to the anatomy to which the base **1022** is connected. The cap engaging portion **1036** can include a portion that binds or engages the base **1026** to drive the engaging members **1028** into a selected portion of the anatomy to assist in resisting rotation of the base **1026**. Further, the base engaging portion **1034** can be keyed relative to the cap engaging portion **1036** to resist rotation or ensure a selected orientation of the cap **1030** relative to the base **1022**. The keyed portion or the anti-rotation feature can be the engaging portion is substantially non-cylindrical and includes a selected geometry.

Further, the base portion **1022** can be used as a fiducial marker. For example, the base **1022** can be fixed to a selected portion of the anatomy of the patient **14** during an imaging process to produce image data. The images can include the image of the base **1022** and the base can be maintained in place prior to and during an operative procedure. Therefore, the base **1022**, such as the cap engaging

portion **1036**, can include a divot or a marking portion that can be used to calibrate the image space to the patient space.

Although the tracking sensor **1022** can be any appropriate tracking sensor, such as that disclosed in U.S. Pat. No. 6,499,488 to Hunter et al. issued Dec. 31, 2002 or U.S. Pat. No. 6,381,485 to Hunter et al. issued Apr. 30, 2002, each of which is incorporated herein by reference, the tracking sensor **1020** can be any appropriate tracking sensor. For example, the tracking **1030** can be substantially a single use member and can snap onto the base **1022**. Further, the cap **1030** can be formed in any appropriate shape for use in the operative procedure. Also, the sensor coils **1032** can be substantially integrally formed to form as a single piece with the cap **1030**, such as molding the coils **1032** within the cap **1030**. Further, the coils **1032** can be substantially wireless or wired. Therefore, it will be understood that a wire may extend from the cap **1030** to interconnect the coils **1032** with the probe sensor **50**. Nevertheless, the cap **1030** can be formed in such a manner to allow it to be only destructively removal from the base **1022**. Therefore, the cap **1030** can be substantially a single use cap for various purposes, such as insuring sterility, insuring operability, and the like.

With reference to FIG. **42**, a tracking sensor assembly **1050** is illustrated, according to various embodiments. The assembly **1050** can include a tracking sensor cap **1052** that can be similar to the cap **1030** in the tracking sensor assembly **1020**. The cap **1052** can include sensor coils (not illustrated) or any other appropriate sensor, such as those discussed above, and can be wired with a wire **1054** or wireless, according to various embodiments. The assembly **1050** can include a connection portion **1056** similar to the connection portion **370** described above. It can, briefly, include a first leg **1058** and a second leg **1060** that can be moved relative to one another with the fixation screw **1062**.

The connection member **1056** can further include a connection post **1064**. The connection post **1064** can include a sensor engaging portion **1066** and an anti-rotation or keyed portion **1068**. The sensor engaging portion **1066** can engage a complimentary portion of the sensor body **1052**. The connection can be a snap engagement such that no other tools are required to interconnect the body **1052** and the post **1064**.

The anti-rotation portion **1068** can also fit or engage with a complimentary portion of the body **1052**. The anti-rotation portion can assist in reducing or eliminating rotation of the body **1052**, and thus the sensors, relative to the connector **1056**. This can assist in increasing the degrees of freedom of tracking that is possible if the sensor and the second body **1052** are fixed relative to the connector **1056**. It will be understood, however, that the anti-rotation portion **1068** can be any appropriate portion. For example, any appropriate geometry, such as a polygon or square, can be used to resist rotation with connection to the body **1052**.

With reference to FIG. **43** a tracking sensor assembly **1080** is illustrated. The assembly **1080** can include a sensor cap **1082** that includes tracking sensors that can be wired with the wire **1084** or wireless, such as those discussed above according to various embodiments. The sensor cap **1082** can be connected to a connector **1086**. The connector can include a threaded body **1088** that can be threaded into bone or any other appropriate portion. The connector **1086** can, therefore, connect the cap **1082** and the sensor (not illustrated) included therein to a selected portion.

The connector **1086** can further include a cap connector portion **1089** that extends from the body. The cap connector **1089** can be similar to the connector **1064** described above. The cap connector can include a cap fixing portion **1090** that

is able to engage and hold a complimentary portion of the cap **1082**, such as that discussed above according to various embodiments. This connection can be a snap connection such that no additional tools are necessary for the connection to be made. Further an anti-rotation portion **1092** can be provided. The anti-rotation portion **1092** can also engage a complimentary portion in the cap **1082**. As discussed above the anti-rotation portion **1092** can be the depression or any other appropriate mechanism or geometry.

Further, it will be understood that the various portions of the tracking sensors according to various embodiments can be formed of selected materials, such as non-magnetic materials including various synthetic materials or non-magnetic alloys. Further the cap or body portions, which can also be referred to as sensor body portions according to various embodiments, can be formed in a manner such that they are single use sensors and are destroyed upon removal from the connecting portions. Moreover, as described above, the snap connections can ease the use of the devices and increase operative efficiency.

This can also allow for of interchangeability. The same sensor body can be moved from instrument to instrument in a selected procedure or from base to base. For example, a sensor body can first be used as a DRF in a selected location on the patient **14** and then moved to a second location. For example, the DRF **50** can be moved from a femur to a pelvis, one vertebrae to another, or from the anatomy to an instrument, etc. The DRF **50**, or appropriate sensors, can also be attached to any portion that can move relative to another. For example, fractured portions of bone can be tracked relative to one another for repairing the bone or placing an implant relative to one another. Also, the sensor body can be moved from a DRF location to an instrument or vice versa. This can decrease cost, inventory, and the number of items in an operating theatre.

Also, in the surgical navigation system, such as the surgical navigation system **10** illustrated in FIG. **1**, the dynamic reference frame **50** can be used to maintain a registration between the patient space and the image space. That is, the dynamic reference frame **50** can be used to insure that the displayed image or coordinates of the patient and the instruments and the relative positions between the two, in image space, are in fact, substantially similar to what is actually occurring between the real instruments and the actual patient, in patient space.

Not only can a registration be formed and maintained between image space and patient space, it can also be formed between the image space and a coordinate system. Alternatively, or in addition thereto, a registration may also be between the coordinate of the patient and a coordinate system. For example, an instrument can be tracked relative to a coordinate system and illustrated on a display, such as the display **34**. The coordinate system can simply be a system that shows a representation of a position of the instrument relative to a position of the dynamic reference frame **50**, or any appropriate reference frame. Therefore, the instrument can be tracked only to a coordinate system, such as an XYZ coordinate system, rather than to a specific image. This can be used for efficiency, positioning of elements in space, and the like. Further, the instrument or the dynamic reference frame **50** can be used to track or localize morphed atlas models, atlas models, to an imageless system, such as one including a coordinate system, or any appropriate system. Therefore, it will be understood that the registration and localization can be done between the patient

space and any appropriate system such as an image, an imaging system, a coordinate system, an atlas model, or the like.

Nevertheless, the dynamic reference frame **50** can be designed according to a selected configuration, geometry, and other considerations for achieving a selected result. Including the various embodiments discussed above and herein. For example, the size and geometry of the dynamic reference frame can be selected to allow for a percutaneous or subcutaneous positioning of tissue over the dynamic reference frame, as discussed briefly above. Various design aspects can also be selected for partial placement through a skin while a portion of the DRF extends above the skin. Nevertheless, the dynamic reference frame can be provided according to various embodiments, including those described further herein. It will be understood, that although reference can be made to a dynamic reference frame (DRF) herein, that the DRF can also be used for any appropriate tracking portion to track any appropriate member, or any portion thereof.

With reference to FIGS. **44-48**, a tracking sensor assembly **1100** is illustrated. The tracking sensor assembly **1100** can be used for any appropriate purpose, such as a dynamic reference frame that is selectively interconnected with a portion of an anatomy, such as a portion of the patient **14**. The tracking sensor assembly **1100** or DRF **1100** generally includes a tracking sensor or coil holding board **1102**, a housing assembly, including a housing lid or upper portion **1104**, and a housing base or lower portion **1106** that is able to surround and hold the board **1102** in a selected position. The housing **1104,1106** can be interconnected with a sleeve **1108** and an anchor or holding member, such as a bone screw **1110**, can be used to hold the housing **1104, 1106** and the sleeve **1108** relative to the patient **14**, when positioned relative thereto. The anchor can also be any appropriate anchor or attachment member, such as, but not limited to, a staple, a rivet, a pin, barb, screw, clamp, crimping onto the bone, combinations thereof, etc.

The dynamic reference frame **1100** can include any appropriate dimensions. For example, from a distal end of the screw to a top of the housing **1104**, when assembled, the DRF **1100** can have a dimension **1112**. The dimension **1112** can be any appropriate size, such as about 10 mm to about 100 mm. Further, the sleeve **1108** can extend from a first end and the assembly **1100** can terminate at a top of the housing **1104** and have a dimension of **1114**. The dimension **1114** can be any appropriate dimension, such as about 1 mm to about 50 mm.

The sleeve **1108**, at a distal end thereof, can include a plurality of attachment portions **1116**. The attachment portions **1116** can be any appropriate portion such as a tooth, plurality of teeth, thread turn or partial turn, an anchor (e.g. the anchors discussed herein), or the like. It will be understood, however, that the attachment portion **1116** can be any appropriate attachment or engagement portion according to various embodiments. The projections **1116** can extend from a second end **1118** of the sleeve **1108**, while a first end **1120** of the sleeve **1108** can be near an exterior of the anatomy of the patient **14** when positioned relative to the patient **14**. The teeth **1116**, or any appropriate projection, can engage a portion of the anatomy, such as a bony portion of the patient **14** to assist in holding the dynamic reference frame **1100** in a selected position. For example, the projections can be used to prevent rotation of the sensor **1100**, as well as to hold and secure the sensor in the X, Y, and Z as well as pitch, yaw, and roll (i.e. six degrees of freedom). Therefore, the dimension

1114 can be the dimension that is substantially equivalent to the distance between the first end **1118** and a second end **1120** of the sleeve **1108**.

The housing including the lower portion **1106** and the upper portion **1104** can surround the board **1102**. The board **1102** can include a plurality of coils, such as inductor portions, conductive portions, or the like. It will be understood that the coils discussed according to various embodiments can be inductive, conductive, combinations thereof or any appropriate coil type. Further the coils can be distinct cold, surface mount coils, or formed in any appropriate manner according to various embodiments.

The coils can, however, include three coils **1122, 1124, and 1126**. Each of the coils **1122, 1124, 1126**, can be positioned on the board **1102** substantially orthogonal to one another or at any appropriate angle relative to one another. The various angles of the sensor coils **1122, 1124, 1126** can be used in various navigation systems to determine a precise location of the DRF **1100**. It will be understood that the board **1102** can also include a battery **1128**, so that the board **1102** is self-powered. Alternatively, or in addition thereto, a power signal can be sent to a component in the board **1102** to provide power to the DRF **1100**. For example an LC tank circuit can be provided or any circuit that can be charged and discharged on the board. It will be understood, however, that according to various embodiments the DRF, such as the DRF **1100**, can be wireless. Further, the various portions of the board **1102** can be substantially hard-wired for both power and a transmission of a signal from or to the DRF **1100**. The wire **1130** can be interconnected with the surgical navigation system, somewhere to the DRF **54** (FIG. **1**).

Although the three coils **1122, 1124, 1126** are illustrated it will be understood that any appropriate number or sets of coils can be used, according to various embodiments described herein, and discussion of coils herein is not limited to a single coil at any location. For example, the DRF can include three sets of two coils, or any appropriate number. Having three coils is not a requirement or a limitation. Also, the coils or sets of coils can be provided at any appropriate angle relative to one another. For example, the coils can be set at about 60 degrees to one another or in any appropriate triangle.

Also, the coils could be any appropriate type of sensor. For example, the coils can also be positioned near a flux gate or the flux gate can be positioned with the coils. Thus, either an AC or DC source can be used to drive the sensor portions, such as the coils or flux gate sensors. It will be understood that the various types of coils, the orientation thereof, the groupings thereof, and the like, can be used in various embodiments described herein. Therefore, reference to the coils herein will also be understood to relate to the various types of coils and orientations thereof described above.

The DRF **1100**, according to various embodiments, including those described herein, can be completely or partially reusable or disposable. For example the anchor can be formed of a material that can be cleaned and/or sterilized for use on multiple different patients. While the housing or body can be formed of a material that is made for a single use and is disposed after the single use.

The board **1102** can be positioned within the housing defined by the upper portion **1104** and a lower portion **1106** in any appropriate manner. For example, the board **1102** can include one or more positioning points, such as an aperture or bore **1132a, 1132b and 1132c**. A member of either or both of the housing portions **1104, 1106** can engage the apertures **1132a-1132c** in the board **1102**. For example, a projection or a plurality of projections **1134a, 1134b, and 1134c** can

project from the lower housing **1106**. The projections **1134a-1134c** can engage the apertures **1132a-1132c** to hold the board **1102** in a fixed position relative to the lower housing portion **1106** and the upper housing portion **1104** to enable precise tracking.

The upper and lower housing portions **1104**, **1106** can be interconnected in any appropriate manner. For example, a snap fit or friction fit can be formed by engaging a projection on one of the portions into a recess of the other portion. Further, or alternatively thereto, the housing portions may define complimentary threads. Nevertheless, the upper housing portion **1104** can be positioned relative to the lower housing portion **1106** to be fixed thereto.

Further, either or both of the housing portions can define a plurality of splines **1136** that can engage a plurality of splines **1138** defined by the sleeve **1108**. The splines **1138** on the sleeve **1108** can engage the splines **1136** on the lower housing portion **1106** to substantially eliminate or resist rotation of the lower housing portion **1106** relative to the sleeve **1108**. This can help insure that the board **1102** also does not rotate relative to the sleeve **1108** and, as discussed briefly above, and described further herein, this can help insure that the board **1102** does not rotate relative to the patient **14** due to the positioning of the screw **1110** through the housing and the sleeve **1108** and the projections **1116**, which can engage the anatomy.

The upper housing portion **1104** can define a bore **1140** through which the screw **1110** can pass. When assembled, the bone screw **1110** can pass through the bore **1140** defined by the housing, a bore **1142** defined by the board **1102**, a bore **1144** defined by the lower housing, and a bore **1146** defined by the sleeve **1108**. It will be understood that each of the bores can cause the respective portions to define a cannula or that the bore is throughbore.

As illustrated in the various drawings, particularly when the screw is positioned and the housing is assembled, the screw **1110** can include an upper washer or abutment portion **1148** that can engage an internal bearing surface **1150** of the sleeve **1108**. This can provide a force onto the sleeve **1108** that can help push or force the projections **1116** into the anatomy. Also, as discussed herein, the screw **1110** can include various other portions or be interconnected with other members to assist in holding it relative to the patient **14** and resist movement once it has been positioned relative to the patient **14**.

The DRF **1100** can be positioned relative to the patient **14** in any appropriate manner. For example, a tool **1152** can be interconnected with a screw head **1154** of the screw **1110**. The tool **1152** can engage the screw head **1154** in any appropriate manner, such as with attracting magnets, a friction fit, an interference fit, or the like. Examples of interference fit screws and tools include the TiMesh™ system sold by Medtronic, Inc. This can allow the screw **1110** to be driven into the patient **14** with a substantially single hand of a user, such as the physician **614**. This can also allow a first user to assemble the tool **1152** and the screw **1110** and pass it to a second user, such as the physician **614**. Such an assembly or assemblance of the portions can be used for various portions, such as passing it from a non-sterile to sterile field, between sterile fields, from a sterilization system to a sterile field, or the like.

The tool **1152** can engage the screw **1110** once it has passed through the housing **1104**, **1106** and the sleeve **1108**. The entire assembly can then be positioned relative to the patient **14** to drive the DRF **1100** into the patient **14**. According to various embodiments, however, the screw **1110** alone can be engaged by the tool **1152** for insertion or

it can be inserted through the sleeve **1108** positioned on a portion of the screw **1110** during the insertion.

The DRF **1100** can be positioned into the patient **14** in any appropriate manner. For example, with particular reference to FIG. **48**, an incision **1160** can be formed in the patient **14**.

The incision **1160** can be formed relative to any appropriate portion of the anatomy, such as the pelvis, a femoral head, a tibia, or any other appropriate portion. A passing tube or cannula **1162** can be positioned through the incision **1160** in any appropriate manner, such is known to one skilled in the art. Further, the incision **1160** can include a stab wound formed by the passing cannula **1160** with a trocar (not illustrated) or any other appropriate portion. Regardless, the passing tube or cannula **1162** can allow the DRF **1110** to be passed through the soft tissue of the patient **14** without substantially engaging or touching the soft tissue of the patient **14**. For example, the passing cannula **1162** may allow for positioning of the DRF **1100** and performing a procedure without requiring suturing the incision **1160**.

Further, the tool **1152** that can be interconnected with the screw head **1154** can ease the insertion of the DRF **1100** by allowing a substantially single handed implantation of the DRF **1100** into the patient **14**. The tool **1152** can also, or alternatively, be interconnected with any portion of the DRF **1100** for a substantially single handed positioning thereof.

As discussed above, driving the DRF **1100** into the patient **14** with the screw **1110** can assist in driving the projections **1116** into the patient to assist in reducing rotation of the housing **1104**, **1106**. Further, or alternatively, or in addition thereto, the screw **1110** can define a cannula or through-bore and a wire, such as K-wire, can be passed through the cannula defined by the screw **1110**. The wire **1170** can exit the screw **1110** in any appropriate position to assist in reducing rotation of the screw **1110** or any portion of the DRF **1100**. The wire **1170** can be keyed relative to the cannula defined by the screw **1110**, such as including a substantially non-circular external circumference. For example, the wire **1170** can be square, octagon, oblong, or the like to substantially assist in reducing or resisting rotation of the screw **1110**. The wire **1170** can also be used to assist in positioning the DRF **1100** relative to the patient **14**, similar to a generally known guide wire, but can also exit the screw or define a barb **1172** that can further engage the anatomy, such as a bony portion to assist in reducing rotation of the screw **1110**.

Further the sleeve **1108** can define a thread at a distal end thereof, such as a partial turn of a thread **1174** to further assist in engaging the bone portion. For example, the turn of thread **1174** can engage the bone during a final rotation or tightening of the screw **1110** into the anatomy of the patient **14**. Thus, the thread **1174** can engage the sleeve **1108** substantially into the bone to assist in reducing rotation of the DRF **1100**.

During insertion of the DRF **1100**, it will be understood that various protective or covering portions can be provided. For example, with reference to FIG. **48**, a protective sleeve or covering **1170** can be provided to cover a portion of the screw **1110**. The covering **1170** can be any appropriate covering, such as a polymer coating, a foil, or the like. The covering **1170** can cover a portion of the screw **1110**, such as a distal end of the screw which may be sharp. The covering **1170** can assist in protecting various soft tissues of the patient **14**, such as skin, muscle, and the like. The covering **1170** can work in cooperation with the cannula **1162** or can be provided when the cannula **1162** is not used. The covering **1170** can be deformable, destructible or the like. For example the covering **1170** can be punctured by the

screw **1110** when it is engaged near a hard surface, such as a bone of the patient **14**. As the screw **1110** is driven into the patient **14**, the screw **1110** can push through the covering **1170** to engage the bone.

Further, a covering or plug can **1172** can be provided near a portion of the sleeve **1108**. The plug or protective portion **1172** can be positioned near an end of the sleeve **1108** while the screw **1110** is positioned more proximally rather than through the sleeve **1108**. The DRF **1100** can then be positioned relative to the patient **14**, similar to that illustrated in FIG. **45B**. However, as the sleeve **1108** engages the bone, the screw **1110** can push through the plug **1172** to engage the bone to assist in holding or fixing the DRF **1100** relative to the bone. Therefore, the plug **1172** can assist in protecting various portions of the patient **14**, such as the skin, the muscle, and other soft tissues from portions of the screw **1110** that may be sharp. The plug **1172** can be used with or separate from the cannula **1162** for various purposes. It will be understood that various other protective portions can be provided, such as having the plug **1172** extend over the projections **1116**. Therefore, the various portions of the DRF **1100** that can be sharp can be covered during positioning of the DRF **1100** relative to the patient **14** until the DRF **1100** engages a hard part of the patient, such as a bone.

It will be understood that various portions of the DRF **1100** can be formed of different materials. It may be selected that the various portions of the DRF **1100** are formed of non-ferrous or non-magnetic materials to assist in resolution of the coils **1122**, **1124**, **1126**. Nevertheless, the various portions of the DRF **1100** can be formed of biologically acceptable metals or metal alloys or polymers. For example, the housing **1104**, **1106** can be formed of polymer materials, so that they are easy to form, can be flexible, if selected, or other selected considerations. For example, the housing portions **1104**, **1106** can be injection molded in any selected shape, size, design or the like. Nevertheless, the substantially radiused edges of the housing **1104**, **1106** can be provided for various reasons, such as aesthetic considerations, reduced friction or engagement of the soft tissue during or after implantation, reduced engagement of the various tools or surgical instruments, or the like. The substantially uniform and radiused geometry can assist in reducing friction or engagement between the housing **1104**, **1106** and the soft tissue, the instruments, or the like to assist in reducing rotation of the DRF **1100**. Further, the aesthetic appeal of the design and the tactile smoothness can also be considerations.

Nevertheless, various portions, such as the screw **1110** can be formed, either completely or partially, of bioabsorbable or resorbable materials. Also, the screw **1110** can include a coating or other portion than can allow for a delivery of a biological active agent, such as a pharmaceutical. For example, during positioning of the DRF **1100** relative to the patient **14**, the DRF **1100** can be fixed relative to the patient **14**. For a removal of the DRF **1100**, however, it can be selected to allow a selected portion of the DRF **1100** to remain in the patient to be resorbed. For example, the retaining washer or abutment washer portion **1148** can be formed to break away at a selected stress, such that the sleeve **1108** and the housing **1104**, **1106** can simply be pulled off of or pulled away from the patient **14** so that the abutment washer **1148** breaks away and the housing **1104**, **1106** and the sleeve **1108** can simply be pulled away from the patient **14**. If the screw **1110** is formed of a resorbable material, it will resorb over a selected period of time and will not cause any discomfort or ill effects to the patient **14**. It will be understood, however, that various other attachment portions

may also be used to affix the DRF **1100** to the patient **14** and they may also be formed of bioabsorbable or resorbable materials. For example, surgical staples, spikes, or the like can be used to affix the DRF **1100** to the patient **14**.

The sleeve **1108**, including the projections **1116** can be positioned relative to a portion of the patient **14**, while allowing for a substantially minimal amount or no amount of preparation of the portion of the anatomy. For example, the sleeve **1108** includes geometry or construction and the projections **1116** that allow the sleeve **1108** to engage a substantially unprepared portion of bone. The sleeve **1108** can easily and efficiently be positioned relative to a bony portion and driven in with a selected amount of force to cause the projections **1116** to engage the bone of the patient **14**, regardless of the underlying geometry of the bone of the patient **14**. Therefore, the bone of the patient **14** need not necessarily be prepared, such as by flattening a bone portion, for engagement by the sleeve **1108**. It will be understood that the various users may select that the bone be prepared or a selected amount of preparation may be selected for various procedures, (e.g. forming a flat surface on the bone) but the sleeve **1108** need not necessarily be used with a prepared bone surface.

Further, as discussed above, the board **1102** can provide or include a selected number of sensor coils. Nevertheless, various other portions of the DRF **1100** can also define or include a plurality of coils. For example, a coil **1180** can be defined on the portion of the screw **1110**, such as on a shank portion of the screw **1110**. The coil **1180** can be provided in addition or supplementary to the coils **1122**, **1124**, **1126** on the board **1102**. Alternatively, the coil **1180** defined on the screw **1110** can replace one or more of the coils on the board **1102**.

The various portions of the DRF **1100** described above with reference to FIGS. **44-48** can be provided according to any of a plurality of various embodiments described below and above, such as the sensor **1020** illustrated in FIG. **41**. Further, the various portions of the dynamic reference frame **1100** can be included in any of the various embodiments of the reference sensors, tracking sensors or the like, described herein, even if they are not specifically described with relation to various embodiments. The omission is not meant to limit the various embodiments, but simply for efficiency of the description and teachings included herein.

With reference to FIGS. **49-53**, a sensor assembly **1200** is illustrated. The sensor assembly **1200** can be used for any appropriate purpose, such as a dynamic reference frame (DRF) for use with the patient **14**. The dynamic reference frame **1200** can be used for any purpose, such as the dynamic reference frames described above according to various embodiments. The dynamic reference frame **1200**, however, can include an attachment member, such as a bone screw **1202**. The bone screw **1202** can include a distal threaded portion **1204**, a proximal sensor body engagement portion **1206**, and an anti-rotation collar **1208**. The anti-rotation collar **1208** can engage a selected portion of a lower housing member **1210**, as discussed further herein.

The lower housing portion **1210** can interconnect with an upper housing portion **1212** to hold a board **1214** in a selected position. The board **1214** can be similar to the board **1102** discussed above. The board **1214** can include one or more coils, such as inductor coils, electromagnetic coils, or the like. The coils **1216**, **1218**, and **1220**, can be positioned relative to each other in any appropriate manner. For example, the coils can be formed around axes that are substantially orthogonal to one another. The board **1214** can also include a battery **1222** to power the board **1214**.

Alternatively, or in addition thereto, the dynamic reference frame **1200** can be wired, such that it includes a hard-wire **1224** for various purposes, such as providing power, transmitting a signal, receiving a signal, or the like. Alternatively, or in addition thereto, a power signal can be provided to various components **1214** for operation of the DRF **1200**.

The lower housing **1210** can include projections **1226**, **1228** that can engage or project through bores **1230**, **1232** defined by the board **1214**. This can allow the board **1214** to be held relative to the lower housing portion **1210** to insure that the board **1214** does not move or has limited movement relative to the base **1210**. The upper housing portion **1212** can engage the lower housing portion **1210** in any appropriate manner. For example, the upper housing portion **1212** and the lower housing portion **1210** can include mating or complimentary threads, a snap fit can be formed between the upper housing portion **1212** and the lower housing portion **1210**, or any other appropriate interconnection can be used. The snap fit can include a groove formed in one of the two housing portions and a complimentary projection formed in the other for a mating engagement.

The lower housing portion **1210** can define a plurality of portions for interconnection with a portion of the screw **1212**. For example, a female receiving port **1238** can be defined by the lower housing portion **1210** to engage the male connection portion **1206** of the screw **1202**. The interconnection can be a snap fit, a threaded fit, or the like to allow for interconnection of the lower housing portion **1210** into the screw **1202**.

The lower housing portion **1210** can also include an anti-rotation recess or female portion **1240**. The anti-rotation recess **1240** can engage the anti-rotation collar **1208** of the screw **1202**. The anti-rotation collar **1208** of the screw **1202** can include any appropriate geometry that can mate with the geometry of the anti-rotation recess **1240** to resist rotation of the lower housing portion **1210** relative to the screw **1202**. For example, as illustrated, the anti-rotation collar **1208** can be substantially triangular. The anti-rotation collar **1208** can then engage a portion of the recess **1240**, such as a depression **1242**. It will be understood that a plurality of the portions of the anti-rotation collar **1208** can engage a plurality of the depressions **1242** defined by the anti-rotation recess **1240**.

As discussed above, the various portions of the DRF **1200** can be formed of selected materials. For example, the lower housing portion **1210** and the upper housing portion **1212** can be formed of a polymer material or any other appropriate material. This may allow the housing **1212**, **1210** to be deformable for various purposes. Further, the screw **1202** can be formed of various metals or metal alloys for interconnection with a selected portion of the patient **14**. Alternatively, the screw **1202** can include various polymer materials that can resorb over a period of time. Thus, the screw **1202** can be left in the anatomy without causing adverse reaction within the anatomy of the patient **14**, due to the fact that it is able to resorb over time.

The DRF **1200** can also include any appropriate dimensions. For example, the screw **1202** can include a dimension **1250** that allows for interconnection of the screw **1202** into a selected portion of the anatomy. However, the housing **1210**, **1212** can include a dimension **1252**. The dimension **1252** can be any appropriate dimension that allows for positioning of the DRF **1200** relative to a selected portion of the anatomy. The DRF, according to various embodiments, therefore, can be low profile to allow soft tissue to pass over the DRF.

It will be understood that a lower portion of the housing **1211** can engage a selected portion of the anatomy, such as the surface of a bone. Therefore, the dimension **1250** of the screw **1202** can be substantially buried in a portion of the anatomy, such as a bone, while the bottom **1211** of the lower housing portion **1210** contacts the bone surface. Therefore, the dimension **1252** of the housing **1210**, **1212** can be any appropriate dimension that is selected to extend beyond a surface of the bone. For example, the dimension **1252** can be about 1 mm to about 50 mm. The dimension **1252** can be selected for various purposes, such as for subcutaneous movement, percutaneous positioning, or the like.

Further, it will be understood that various portions of the housing **1210**, **1212** can be substantially rounded or radiused for various purposes. For example, the radiused edges can help minimize tissue disturbance during positioning of the DRF **1200**, movement of the DRF **1200** relative to soft tissue during a movement of the anatomy, or any other appropriate reason. Further, a top **1213** of the upper housing portion **1212** can include a selected radius for minimization of contact or disturbance of the soft tissue or contact with various surgical instruments.

It can be selected that the dimensions and geometry of the housing **1212**, **1210** can be selected for movement about soft tissue. For example, the DRF **1200** can be positioned below soft tissue and relative to a bone portion. Then, when the bone is moved the DRF **1200** can move relative to the soft tissue without substantially damaging the soft tissue, hindering movement of the bone portion relative to the soft tissue, or the like.

Although discussed in detail above, the DRF **1200** can include features substantially similar to the DRF **1100** discussed above. For example, the screw **1202** can be cannulated, as can the portion of the housing **1210**, **1212** for positioning of a guide wire or wire therethrough. As discussed above, the wire can include a portion that is keyed relative to the screw **1202** and/or the housing **1210**, **1212** to resist rotation relative thereto and can include a barb to engage the anatomy.

Further, the DRF **1200** can be passed through an incision **1260** in the patient **14**. However, the DRF **1200** can be implanted in any appropriate manner. For example, a tool can interconnect with any portion of the screw **1202**, such as the anti-rotation collar **1208** and the housing can engage portion **1206** to pass the screw **1202** through a cannula **1262** that can be positioned through the incision **1260**. The tool can engage the housing engagement portion **1206** substantially similar to the housing **1210**. Therefore, the screw **1206** can be efficiently held relative to a tool for manipulating the screw **1202**.

The screw **1202** can be inserted into the anatomy, such as a bone portion, to any appropriate depth. Once the screw **1202** is inserted a selected length, such as by twisting the screw **1202**, the tool can be disengaged by removing it from the engagement portion **1206**, due to the resistance by the threads engaging the bone. It is optional to position relative to the anti-rotation flange a protective washer or sleeve **1270**. The protective washer or sleeve can be formed of any appropriate material, such as a bioresorbable or resorbable material. The tissue protective washer **1270** can assist in reducing interaction between the various portions of the screw, such as the anti-rotation flange **1208**, and the soft tissue of the patient **14**. This can assist in minimizing the trauma during a surgical procedure.

The housing **1210**, **1212**, that can be pre-assembled or assembled during its positioning relative the screw **1202** can also be passed through the cannula **1262** to engage the

engaging portion **1206**. Thus, it will be understood that the DRF **1200** can be implanted in any appropriate manner. It can allow for positioning of the screw **1202** relative to a selected portion of the anatomy and then engaging the engagement portion **1206** with the housing **1210**. As discussed above, the various portions can resist rotation of the housing **1210** and the board **1214** relative thereto, due to the interconnection therewith. Therefore, the housing **1210**, **1212** can be held in a relative orientation to the screw **1202**.

It will be understood that the various features described above and herein can be applied to the DRF **1200** even though not specifically described. Further, the DRF **1200** can be positioned relative to any appropriate portion of the anatomy, such as a femur (e.g. greater trochanter), a pelvis (e.g. the iliac crest), the tibia, the humerus, or the like. It will be understood that the DRF **1200** can be positioned relative to any appropriate portion of the anatomy for use of the DRF **1200**.

With reference to FIGS. **54-58**, a sensor assembly **1300** is illustrated. The sensor assembly **1300** can be used for any appropriate purpose, such as a DRF, similar to the DRF **54**. The dynamic reference frame **1300** can include any appropriate portions, such as an anchor portion, which can include a screw **1302**. A lower housing portion **1304** and an upper housing portion **1306** can surround and enclose a board **1308**. The housing portions **1304**, **1306** can be positioned through or into a sleeve **1310**.

The sleeve **1310** can include a lower portion **1312** and a projection **1314** that extends from the lower portion **1312**. The projection **1314** can be similar to the projection **1116** described above. The projection **1314** can engage a selected portion of the anatomy, such as a bony portion for resisting rotation of the sleeve **1310** relative to the anatomy.

The screw **1302** can include a lower portion defining a thread **1316**. According to various embodiments, the screw **1302** can be completely or partially resorbable or formed of any appropriate material. An upper portion can include a tool engaging portion **1318** and a washer or flange **1320**. During insertion of the screw **1302** through the sleeve **1310**, the flange **1320** can engage the sleeve **1310** in any appropriate manner to allow for a force to be transferred from the screw **1302** to the sleeve **1310**. Further, the flange **1320** can act as a lock washer to resist rotation between the sleeve **1310** and the screw **1302** during and after positioning of the screw **1302** through the sleeve **1310**.

Further, the sleeve **1310** can be formed as a single member with the screw **1302**. Also, the screw **1302** can be any appropriate anchor portion (e.g. a staple, a pin, a wire, a rivet, etc.), which allows for anchoring the sleeve or the DRF **1300** relative to a selected portion of the anatomy. Nevertheless, the screw **1302** and the sleeve **1310** can be formed as a single member for efficiency or positioning of the DRF **1300** relative to the patient **14** or for other appropriate purposes.

The board **1308** can include a portion similar to the board **1214** or other boards described herein. For example, the board **1308** can include a sensing coil or a plurality of sensing coils **1324**, **1326** and **1328**. The coils can be formed in any appropriate manner and can be formed substantially orthogonally to one another or define axes that are orthogonal to one another. The sensing coils can be electromagnetic coils or induction coils. Further, a battery **1330** can be included for powering the board **1308**. Alternatively, or in addition thereto, a wire **1332** can be provided to provide power, transfer a signal or the like between the board **1308** and other portions of the assembly. Further, as discussed above, a power signal can be provided to the board **1308**.

The board **1308** can be positioned within the lower housing portion **1304** in any appropriate manner. For example, the lower housing portion can define a first track or passage **1334** and a second track or passage **1336** into which the board **1308** can be positioned. The board **1308** can be positioned between the two tracks **1334**, **1336** to assist in holding the board **1308** relative to the lower housing portion **1304**. The two tracks **1334**, **1336** can assist in holding the board **1308** in a selected position within the lower housing position **1304**.

The lower housing portion can also define a connection portion, which allows it to interconnect with the upper housing portion **1306**. For example, complimentary threads can be defined on the lower housing portion **1304** and the upper housing portion **1306**, a snap interconnection can be formed between the two, or any other appropriate interconnection can be formed, including those discussed herein according to various embodiments.

The lower housing portion **1304** can also define an engagement region **1340**, which can engage an engagement region **1342** of the sleeve **1310**. The lower housing portion **1304** can snap into the sleeve **1310**, include a complimentary thread, or any other appropriate connection portion, such as an adhesive. Further, the lower housing portion can define a projection **1344** that can interconnect or interact with a passage or recess **1346** defined in the sleeve **1310**. The interconnection of the projection **1344** of the lower housing portion **1304** and the recess **1346** of the sleeve **1310** can assist in reducing or resisting rotation between the lower housing portion **1304** and the sleeve **1310** and also the board **1308** relative to other portions of the DRF **1300**.

The DRF **1300** can include appropriate dimensions, such as those discussed above.

Nevertheless, the lower portion **1312** is generally able to connect or touch a selected portion of the anatomy, such as a surface of the bone. Therefore, a top **1307** of the DRF **1300** can extend the dimension **1350**. The dimension **1350** can be any appropriate dimension, such as the dimensions described above, or those understood by one skilled in the art. Further, it will be understood that the various portions of the DRF **1300** can include any appropriate geometries. For example, many of the portions of the DRF **1300** can be provided with substantially radiused edges to reduce interference contact with the soft tissue. Also, the dimension **1350** can be used to position the selected portion of the DRF **1300** at a selected position relative to the patient **14**.

The DRF **1300** can be positioned relative to the patient **14** in a manner similar to those methods described herein. For example, a cannula **1354** can be used to pass each of the portions of the DRF **1300** through an incision **1356** formed in the patient **14**. It will be understood, however, that the sleeve **1310** and the screw **1302** can be first positioned relative to a portion of the patient **14**.

As discussed above, the screw **1302**, or any other appropriate anchor portion, and the sleeve **1310** can be formed as a single member for efficiency of positioning relative to the patient **14**. Nevertheless, even as separate members, a tool can interconnect with a tool engaging portion **1318** of the screw **1302** to be positioned relative to the patient **14**. As discussed above, a friction fit or other appropriate interconnection can allow for the screw **1302** to be held relative to the tool for manipulation of the screw **1302** with a single hand. Further, the sleeve **1310** can be positioned relative to the screw **1302** prior to positioning the screw in the patient **14**. Therefore, the interconnection between the tool and the screw **1302** can allow for manipulation of the sleeve **1310** as well.

Nevertheless, the screw **1302** can be inserted a selected depth into the patient **14** and can allow for connection or interaction of the projection **1314** with a selected portion of the anatomy, such as a surface of the bone. Nevertheless, the bone can be either prepared or unprepared in any appropriate manner for receipt of the DRF **1300**. For example the bone surface can be flattened or left in a natural state.

Once the screw **1302** and the sleeve **1310** have been positioned, the housing assembly, including a lower housing portion **1304**, the upper housing portion **1306**, and the board **1308** can be fit into the sleeve **1310**, such as with a snap fit, a friction fit, or other connection. This can allow the DRF **1300** to be positioned relative to the anatomy of the patient **14** in any appropriate manner and as a separate or plurality of portions, or as a less number of portions, such as if the sleeve **1310** and the screw **1302** are formed as a single member.

It will be understood that the portions described herein, such as the positioning techniques, the interconnection, or the like can be applied to the DRF **1300** even though not specifically described here. Nevertheless, one skilled in the art will understand that the DRF **1300** can be used with a plurality of instruments or positioning techniques.

With reference to FIGS. **59-69**, a sensor assembly **1400** is illustrated. The sensor assembly **1400** can be a DRF **1400**, for uses similar to the DRF **54**. The DRF **1400** can include any appropriate portions, such as a lower housing portion or base **1402**, an upper housing portion or top **1404**, an anchor, such as a screw **1406**, and a sensor or a plurality of sensor coils **1408**, **1410**, **1412**. The coils **1408**, **1410**, **1412** can be positioned on the base **1402** or on the top **1404** in any appropriate manner. For example, the coils **1408-1412** can be positioned, such that they include axes that are substantially orthogonal to one another. Further, a battery or power cell **1414** can be included in the DRF **1400**, to provide power to the sensors **1408-1412**. Alternatively, or in addition thereto, the DRF **1400** can include a wire **1416**, such that it is hard-wired to a selected portion of the navigation system. Further, the DRF **1400** can include or be used with a power signal that is operable to provide a power signal that is operable to provide power to the DRF **1400** for receiving a signal, sending a signal, and the like.

The housing top **1404** can engage the housing base **1402** in any appropriate manner. For example, a snap fit, a friction fit, or complimentary threads can be formed between the housing top **1404** and the housing base **1402**. This can allow for the housing **1402**, **1404** to be formed relative to the portions that are positioned within the housing **1402**, **1404**, such as the battery **1414** and the sensors **1408-1412**.

The screw **1406** can pass through a bore **1418** defined by the lower housing portion and a bore **1420** defined by the upper housing portion **1404**. The upper housing portion **1404** can further define a recess **1422** that can complement a portion of the screw **1406**, such as a head **1424** of the screw. The complimentary geometry can include a key geometry, such that the upper housing portion **1404** resists rotation relative to the screw **1406**. Because the housing lid **1404** engages the housing base **1402**, the resisting of rotation between the screw **1406** and the housing lid **1404** can also resist rotation of the lower housing portion **1402**.

Further, projecting from a portion of the lower housing portion **1402** can be a projection or a plurality of projections **1426**. The projections **1426** can be bone engaging projections that engage or project into a selected portion of bone once the DRF **1400** is positioned in the patient **14**. Therefore, the screw **1406** can be passed through the housing portions **1404**, **1402** and provide a force to push the pro-

jections **1426** into a portion of the bone to allow for the resisting of rotation between the lower housing portion **1402** and the bone, which can also, because of the interconnection of the screw **1406** and the upper housing portion **1404**, resist rotation of the entire DRF **1400**.

The screw **1406** can include a tool engaging portion **1428**. The tool engaging recess **1428** of the screw **1406** can allow a tool **1430** to engage the screw **1406**. The tool **1430** can interact, such as with a friction interaction, with the tool engaging recess of the screw **1406** so that the DRF **1400** can be implanted with a single hand of a user, such as a physician.

As described above according to various embodiments, the DRF **1400** can be passed through an incision in any appropriate manner, such as with a cannula, tube, or the like. Further, due to the interconnection of the tool **1430** with the screw **1406**, the DRF **1400** can be manipulated with a single hand. Alternatively, the DRF **1400**, or DRF of any of the various embodiments can be manipulated and/or implanted with a robot arm or appendage. A friction fit can be formed between the recess **1422** and the upper housing portion **1404** in the head of the screw **1424** so that the entire DRF assembly **1400** is held together for manipulation with the tool **1430**.

Further, as discussed above, the screw **1406** can be cannulated for use with a guide wire or a keyed wire to further resist rotation of the screw **1406**, and therefore the DRF **1400**, after implantation of the DRF **1400**.

The DRF **1400** can include a selected dimension **1434**. The dimension **1434** can extend from an upper portion **1405** of the housing top **1404** to a lower portion **1403** of the housing base **1402**. The dimension **1434** can be any appropriate dimension, for example, about 1 mm to about 50 mm. The dimension **1434** can be any appropriate dimension that can be similar to the dimensions above or any other appropriate dimension. Nevertheless, the dimension **1434** can allow for positioning of the DRF **1400** relative to a selected portion of the anatomy, such as a pelvis, a femur, a vertebrae, humerus, tibia, or the like. Further, dimension **1434** can allow for minimal contact or interaction with soft tissue during positioning of the DRF **1400**, movement of soft tissue relative to the DRF **1400**, or any other appropriate reason. Further, the housing **1402**, **1404** can include a selected geometry to allow for reduced interaction with the soft tissue, reduce interaction between the DRF **1400** and various instruments, and for other reasons.

With reference to FIGS. **64-68**, a DRF **1500** is illustrated. The DRF **1500** can include a plurality of portions, such as an anchor member, which can be a screw **1502**, an upper housing portion **1504**, and a lower housing portion **1506** can be connected to form a housing member. The housing member can house a plurality of sensor coils, such as a sensor coil **1508**, and sensing coil **1510**, and a sensing coil **1512**. Also, a battery **1514** can be provided to provide power to the DRF **1500**, such as for receiving and transmitting a signal. Further, alternatively, or in addition to the battery **1514**, a wire **1516** can be provided to transmit or receive a signal, provide power to the DRF **1500**, or any other appropriate reasons. Further, as discussed above, a power signal can be provided to the DRF **1500**.

The housing base **1506** can define one or a plurality of tooth bores **1520**. The tooth bores **1520** can receive one or a plurality of teeth **1522**. The teeth **1522** can engage a portion of the patient **14**, similar to the projections as described according to various embodiments. The teeth **1522**, however, can be formed as members separate from the base housing **1506**. It will be understood that the teeth **1522**

may also be formed as a single member with the lower housing **1506**. Nevertheless, the teeth **1522** can be interconnected with the base housing **1506** through an appropriate connection in the bores **1520**. For example, complimentary threads can be formed on the teeth **1522** and in the bores **1520**, a friction fit (e.g. a taper), or other appropriate interconnections can be provided. Further, the teeth **1522** can be provided in different sizes and interconnected by a user during an operative procedure. Therefore, the size, the number, the geometry, and other considerations of the teeth **1522** can be selected by a user during an operative procedure.

The base **1506** can further define an anchor bore **1524** that can be aligned with an anchor bore **1526** defined by the upper housing **1504**. The respective bores **1524**, **1526** can be aligned when the upper housing **1504** is fit to the lower housing **1506**. The housing **1504**, **1506** can interconnect in any appropriate manner, such as with a friction fit, including a snap fit, a respective thread or the like. Further tabs and/or projections can be defined by either portion of the housing, **1504**, **1506** and engage respective slots, or recesses, or the like in the other housing portion (i.e. a snap fit).

The anchor, including the screw **1502**, can include a threaded region **1528** and a tool engaging head **1530**. The tool engaging head **1530** can be used to engage the screw **1502** by a tool for positioning the DRF **1500** relative to the patient **14**. The tool can frictionally engage the head **1530** in a manner that allows a user to manipulate the DRF **1500** with a single hand. Therefore, the DRF **1500** can be implanted with the tool **1532** in an efficient manner.

Further, the DRF **1500** can be positioned through a cannula, an incision, or the like relative to the patient, according to various embodiments, including those described herein. Further, the screw **1502** can be cannulated to allow for passing a wire, such as a keyed guide wire, through the screw **1502** to assist in positioning the DRF **1500** and reducing or resisting rotation of the screw **1502** within the patient **14** after implanting the DRF **1500** therein.

With reference to **65B**, a protective element or member can include the spike **1522** initially provided substantially above a surface of the lower housing **1506**. It will be understood that a biasing member, such as a spring, including a metal coil, a polymer coil, a rubber sleeve, or the like, can be provided to assist in biasing the spike **1522** within the housing assembly. Nevertheless, the spike **1522** can be provided so that substantially no selected portion of the spike **1522** extends below the lower housing **1506** to engage a portion, such as selected soft tissue portions, of the patient **14** until selected. For example, the screw **1502** can include a flange or collar **1560** that can engage the spike **1522** at a selected time. The flange **1560** can engage a top portion of the spike **1522** as the DRF **1500** is driven into the patient **14** as the lower housing **1506** abuts a selected portion of the patient **14**, such as a bone thereof, the screw **1502** can be further driven into the patient **14** therefore allowing the flange **1560** to engage the spike **1522** and drive the spike **1522** into the patient. Therefore, the spike **1522** can be limited in its contact with selected portions of the patient **14** during positioning of the DRF **1500** relative to the patient **14**. Because the spike **1522** is positioned substantially within the housing during the initial positioning of the DRF **1500** relative to the patient **14**, the spike **1522** can be limited in its contact with other portions of the patient **14**, such as selected soft tissues. Further, it will be understood that the various protective elements described herein can be used with any various embodiments of the DRF. Therefore, even if a

particular protective element is not described with it, it can be understood that it can be used for the various embodiments.

According to various embodiments, such as exemplarily illustrated in FIG. **64**, a positioning element **1505** can be provided with a DRF **1500**, or any DRF according to various embodiments. The positioning element **1505** can be any appropriate portion, such as a depression defined by the housing, a projection defined by the housing, a surface structure defined by the housing, or the like. It will be understood that the positioning element **1505**, according to various embodiments, can be formed integrally with the DRF, can be formed as a single member with a portion of the DRF, or in any appropriate manner. However, the positioning element **1505** can assist in positioning, such as implanting or removal, of the DRF. The positioning element **1505** can be engaged by selected tools, a hand of the user, or in any appropriate manner to assist in positioning the removal of the DRF **1500**. Further, the positioning element **1505** can be used in concert with the tool that engages the head **1530** or in any other appropriate manner. It will be understood, however, that the positioning element can be used with any appropriate of the various embodiments and can be any appropriate portion to assist in implanting, removal, or the like of the DRF according to various embodiments.

The DRF **1500** can include any appropriate geometry, such as a substantially radiused or annular geometry. The radiused geometry can assist in reducing interaction with soft tissue, other instruments, or the like during a procedure. Therefore, rotation of the DRF **1500** can be further reduced by reducing contact or interaction of the DRF **1500** with other anatomical or instrument portions.

Further, the housing **1504**, **1506** can define a dimension **1540** that is any appropriate dimension. The dimension **1540** can extend between a top **1505** of the upper housing portion and a bottom **1507** of the lower housing portion **1506**. The bottom **1507** of the lower housing portion **1506** can contact a selected portion of the anatomy, such as a surface of the bone. The dimension **1540**, however, can be any appropriate dimension for various purposes, such as reducing interaction with soft tissue, allowing movement of a bony portion relative to soft tissue without or reducing trauma to the soft tissue or any other appropriate purpose. Therefore, the dimension **1540** can be any appropriate dimension, for example, about 1 mm to about 50 mm.

Further, as discussed above, the DRF **1500** can be formed of any appropriate materials. For example, the screw **1502** can be formed of a substantially bioresorbable or resorbable material for allowing resorption of the screw **1502** at a selected rate. Therefore, the DRF **1500** can be implanted, according to various embodiments and the housing **1504**, **1506** can be removed by breaking away a portion of the screw **1502**, while the remaining portion of the screw **1502** remains in the patient **14** to be resorbed at the selected rate. The screw may also be formed of other materials, such as metals, metal alloys, or other appropriate materials.

Further, the housing **1504**, **1506** can be formed of any appropriate material. For example, the housing **1504**, **1506** can be formed of selected polymer or other resiliently deformable materials. The housing **1504**, **1506** can be formed of a deformable material so that it can mate or conform with a selected portion of the patient, such as a surface of a bone, without the surface of the bone being substantially prepared. Further, the teeth **1522** can include a dimension that allows the housing base **1506** to not be positioned on a substantially flat or non-flat portion of the bone and the teeth **1522** are able to engage the bone in a

manner that substantially resists rotation of the housing **1504**, **1506** after positioning of the anchor in the bone.

With reference to FIGS. **69-73**, a sensor assembly **1600** is illustrated. The sensor assembly **1600** can be used as a DRF, such as the DRF **54** for various purposes. The DRF **1600** can include various portions, that may be formed as a plurality of modular portions or as a single portion, based upon various considerations. Nevertheless, the DRF **1600** can generally include a lower housing portion **1602**, an upper housing portion **1604**, one or a plurality of coils, such as sensor coils **1606**, **1608**, **1610**, an insert **1612**, and an anchor, such as a screw **1614**. The DRF **1600** can also include a battery or other power cell **1616**. Alternatively, or in addition thereto, a wire **1618** can be provided to provide power to the DRF **1600**, transfer a signal to or from the DRF **1600**, or for various other purposes. In addition, or alternatively thereto, a power signal can be provided to the DRF **1600** as is understood by one skilled in the art.

The sensor coils **1606-1610** can be interconnected with the DRF **1600** in any appropriate manner. For example, the coils **1606-1610** can be fixed to the housing portions **1602**, **1604** in any appropriate manner. Also, the coils **1606-1610** can be formed in the housing or as a single member with the housing. Also, according to various embodiments the one of more of the coils **1606-1610** can be formed on or as part of the screw **1614**.

The inserts **1612** can interconnect with a portion of the housing **1602**, **1604**, such as a sidewall **1620** defining a bore **1622**. The sidewall **1620** can also define a key portion **1624** that can interconnect with a complimentary key portion **1626** on the insert **1612**. The insert **1612** can also define a sidewall **1628** that defines the key portion **1626**. The sidewall **1628** can define a bore **1630** that can complement or allow for passage of the anchor **1614** therethrough. The upper housing portion **1604** can also define a bore **1632** for passage of the anchor **1614**.

The anchor **1614** can include a threaded portion **1634**, a tool engaging portion **1636**, and a flange **1638**. The tool engaging portion **1636** can engage a selected tool to allow for insertion of the anchor **1614** and the DRF **1600** relative to a portion of the patient **14**. According to various embodiments, the tool can engage the tool engaging portion **1636** in any appropriate manner. For example, the tool can form a friction fit or the like to allow for interconnection or efficiency of implantation of the DRF **1600**. The tool **1640** can allow for substantially single-handed implantation or positioning of the DRF **1600** relative to the patient **14**.

Extending from a bottom **1642** of the insert **1612** can be one or a plurality of projections **1644**. The projection **1644** can engage a portion of the patient **14**, such as a bony portion. The projection **1644** can extend into or engage a portion of the patient **14** to assist in resisting rotation of the insert **1612** relative to the patient **14**. As illustrated, the flange **1638** of the screw **1614** can press against a flange **1646** of the upper housing **1604** and a top portion **1648** of the insert **1612** defined by the sidewall **1628**. The force of the flange **1642** of the screw **1614** on the various portions can assist in holding the housing **1604**, **1602** relative to the insert **1612**, which can engage the bone through the projection **1644** to assist in resisting rotation of the DRF **1600** relative to the patient **14**. Therefore, the DRF **1600** can be held relative to the patient **14** in a selected manner and in an appropriate orientation and position.

Further, the housing **1604**, **1602** can include any appropriate dimension **1650**, such as those described above. The dimension **1650**, however, can be any appropriate dimension that extends from a top **1605** of the upper housing portion

1604 to a bottom **1603** of the bottom housing portion **1602**. The dimension **1650**, although it can be any appropriate dimension, can be, for example, about 1 mm to about 50 mm.

The dimension **1650** of the DRF **1600** can be selected for various appropriate reasons, such as ease of positioning the DRF **1600** relative to the patient **14**, reducing interaction with the soft tissue of the patient **14**, allowing the DRF **1600** to move subcutaneously or percutaneously on the patient **14**, or other appropriate reasons.

It will be understood, however, that the various portions of the DRF **1600** can be formed as single portions. Although the insert **1612** is shown separate from the housing **1602**, it will be understood that the portions can be formed as a single member. Nevertheless, the insert **1612** being separate from the housing **1602** can allow for selection of the insert **1612** for various purposes. For example, the size of the projection **1644**, the material of the insert **1612**, and other considerations can be chosen, for example, intraoperatively, for various purposes.

Further, as discussed above, the portions of the DRF **1600** can be formed of any appropriate materials, for example, the screw **1614** can be formed of any appropriate materials, such as metal alloys, polymers, or the like. According to various embodiments, the screw **1614** can be formed of a resorbable material, such that the housing **1602**, **1614** can be removed by a breaking away portion of the screw **1614** while the remaining portion of the screw **1614** resorbs into the patient **14** at a selected rate. Further, as discussed above, the screws **1614** can be any appropriate anchor and a screw, as illustrated here, is merely exemplary.

With reference to FIGS. **74-78**, a tracking sensor assembly **1700** according to various embodiments is illustrated. The tracking sensor **1700** can be used for any appropriate purpose, such as a DRF, similar to the DRF **54**. The DRF **1700** can include a plurality of portions, such as a base or lower housing portion **1702**, an upper housing portion **1704**, and a plurality of sensor coils **1706**, **1708**, **1710**. As described above, the sensor coils **1706-1710** can be interconnected with the housing portions **1702**, **1714** in any appropriate manner. Further, the sensor coils **1706-1710** can be inductor coils or can be any appropriate type of coils that are oriented in a selected manner. For example, the plurality of coils **1706-1710** can define axes that can be positioned substantially orthogonally to one another in the DRF **1700**. Further, a battery or power cell **1712** can be provided to provide power to the DRF **1700**. Alternatively, or in addition thereto, a wire **1714** can be provided to provide power to the DRF **1700**. As discussed above, however, the DRF **1700** can be powered by a power signal.

The DRF **1700** can further include a plurality of teeth or spikes **1716**. The teeth **1716** can be similar to the teeth **1622** described above. The teeth **1716** can be received or interconnected with a bore **1718** defined by the lower housing portion **1702**. The teeth **1716** can interconnect with the bore **1718** in any appropriate manner, such as those described above and, as such, will not be described in detail here.

The lower housing **1702** defines a bore **1720** that can allow an anchor, such as a screw **1722** to pass therethrough. The upper housing portion **1704** can also define a bore **1724** for the anchor **1722** to pass through. The bore **1724** can be defined by a sidewall **1726** of the upper housing portion **1704** that can interact with an arcuate or otherwise radiused head portion **1728** of the screw **1722**. The screw can also include a thread **1730** and a tool engaging portion **1732**.

The arcuate head portion **1728**, however, can interact with the sidewall **1726** defined by the upper housing portion **1704**

in a selected manner to allow the screw 1728 to be positioned at an angle relative to a central axis defined by the housing 1704. The central axis 1732 of the upper housing 1704 can be a central axis thereof. The screw 1722, although it can be positioned at any appropriate angle relative to the central axis 1732, it can define a central axis 1734 that can be positioned at an angle 1736 relative to the central axis 1732 of the upper housing portion 1704. The angle 1736 can be any appropriate angle, for example it can range from about 0° to about 90°.

The screw 1722 can be angled relative to the housing 1704 for any appropriate reason. For example, it may be selected to interconnect to the DRF 1700 with a selected portion of the anatomy, but not allow the screw 1722 to intersect or pass through a selected portion of the anatomy. For example, if the DRF 1700 is positioned relative to a long bone, it can be selected to angle the screw 1722, such that the screw does not pass the cortical bone portion and intersect the intramedullary canal of the long bone. It will be understood, however, that the screw 1722 can be angled relative to the housing 1704 for any appropriate purpose.

Further, the housing 1702, 1704 can be interconnected in any appropriate manner, including those described above. For example, the housing portion 1702, 1704 can define complimentary threads, friction fit portions (e.g. snap fit), or any other appropriate interconnection. It will be understood that the housing portions can be interconnected either pre-operatively or intraoperatively.

Further, as discussed above, the teeth 1716 can be selected intraoperatively for various reasons. For example, the teeth 1716 can be selected for a length, a diameter, or the like for interconnecting with a selected portion of the anatomy.

Further, the DRF 1700 can be positioned relative to the anatomy as a single unit due to interconnection of the screw 1722 with the housing portion 1704, 1702. Further, a tool 1740 can engage and frictionally or otherwise hold the screw 1722 for positioning the DRF 1700 with a single hand of a user. Further, as discussed above, the DRF 1700 can be passed through a cannula 1742, passed through an incision, or otherwise positioned in the anatomy of the patient 14.

With reference to FIG. 75B, a protective element according to various embodiments can be provided around the projections for spikes 1716. The protective element can include a compressible or crushable sleeve 1750. The crushable sleeve 1750 can be formed of any appropriate material such as a metal foil, a polymer material, or the like. The compressible sleeve 1750, however, can crush or deform when the screw 1722 is driven into a selected portion, such as a bone of the patient 14, and the protective sleeve 1750 engages the bone. As the screw 1722 is further driven into the bone, the protective sleeve 1750 can compress, if selected, and the spike 1716, however, will not compress. Therefore, as the screw 1722 is driven further into the bone, the compressible sleeve 1750 is pushed up while the spike 1716 is driven further into the bone. Therefore, as discussed above, the spike 1716 can be protected from contacting various portions of the patient 14, such as soft tissues, or other instruments. It will be understood that the screw 1722, can also include a selected protective element.

Further, the crushable sleeve 1750 can include a portion that covers each of the plurality of the spike 1716, as illustrated in FIG. 75B. It will be understood that the crushable sleeve 1750 can be formed as a single portion with the lower housing 1702, formed as a separate member thereof, or the like. Further, the crushable sleeve 1750 can include a bottom portion or extend past the end of the spike 1716.

Further, a single piece protective member 1752 can include a plurality of protective portions 1754 to protect each of the spikes 1716 defined by the DRF 1700. The separate protective elements 1752 can also be formed as a separate member to be fit over the screw 1722 and the projection 1716 or can be formed integrally with the housing 1702, or as a single piece with the bottom housing 1702. The protective member 1752, however, can include substantially similar characteristics to the protective sleeve 1750. That is, each of the protective elements 1754 can be crushed or deformed as the DRF 1700 is driven into the bone. Nevertheless, the protective elements 1752 can be provided for various purposes, such as manufacturing efficiency, assembly efficiently, or the like.

Further, a protective element or member can include a retractable sleeve 1760, as illustrated in FIG. 75C. The retractable sleeve 1760 can be formed of any appropriate material, such as a metal alloy, a polymer, or the like. The protective sleeve 1760, however, is generally rigid. A deformable member or a biasing member, such as a spring 1762 is provided to bias the protective sleeve 1760 in a direction, such as a direction that would cover the spike or tooth 1716. Again, as the DRF 1700 is driven into the patient 14, the protective sleeve 1760 can engage the bone and as the sleeve DRF 1700 is further driven into the patient 14, the sleeve 1760 can push against the biasing member 1762 and expose the spike 1716. Therefore, the spike 1716 would be substantially covered by the protective sleeve 1760 until such time as the spike 1716 is driven into the bone. It will be understood, however, that the biasing member 1762 can be any appropriate member and is not necessarily limited to a spring. For example, a rubber spring, a resilient member, or the like, can be provided to bias the protective sleeve 1760 in a selected direction.

It will be understood that the various protective members, can be used in the various embodiments whether particularly described or not. The protective elements such as the crushable sleeve, the biased sleeve, the crushable member, or the like, can be provided in the various embodiments to reduce the contact between various portions of the DRF, according to various embodiments, and selected portions of the patient 14.

Further, the DRF 1700 can include a dimension 1750 that is any appropriate dimension, including those described above. The dimension 1750 can extend from a bottom 1701 of the lower housing portion 1702 to a top 1705 of the upper housing portion 1704. Although the dimension 1750 can be any appropriate dimension, it can for example, be about 1 mm to about 50 mm.

As discussed above, the DRF 1700 can be formed of various materials, including polymers, metals, metal alloys, or the like. Further, various portions of the DRF 1700 can be formed of various different materials. According to various embodiments, the screw 1722 can be formed of a resorbable material to allow the housing 1704, 1702 to be broken away from the screw 1722 after a procedure so that the screw 1722 can resorb into the patient 14.

It will also be understood that various other specific features can be included in the DRF 1700, that are not specifically described here. For example, the screw 1722 can be cannulated, such that a guide wire can be passed through to assist in reducing rotation of the screw 1722.

Further, the housing 1702, 1704 can be formed of selected materials that allow it to deform or conform to selected portions of the anatomy. Therefore, the DRF 1700 can be positioned relative to a bone surface without substantially preparing the bone surface prior to positioning the DRF

1700 relative thereto. Further, the teeth 1716 can assist in engaging the patient 14 without providing a substantially prepared or flat surface of the bone.

With reference to FIGS. 79-84, a tracking sensor assembly 1800 is illustrated. The tracking sensor 1800 can be used for any appropriate purpose, such as a DRF, similar to the DRF 54 described above and for various purposes, including those described above. The DRF 1800 can include any appropriate portions, such as a lower housing portion 1802, an upper housing portion 1804, and one or a plurality of sensor coils 1806, 1808, 1810. The sensor coils 1806-1810 can be positioned relative to the housing portions 1802, 1804 in any appropriate manner. For example, the sensor coils 1806-1810 can define axes that are positioned substantially orthogonally to one another within the housing portions 1802, 1804. The tracking sensor 1800 can further include a battery or power cell 1812 to provide power to the DRF 1800. Also, as discussed above, a wire 1814 can provide power, signal transmission, or other purposes to the DRF 1800. In addition, or alternatively thereto, a power signal can provide power to the DRF 1800 for various purposes.

The DRF 1800 can further include an anchor 1816 that can be a screw that includes a thread 1818, a radiused or polyaxial head 1820 and a tool engaging portion 1822. The polyaxial head 1820 can allow for the screw 1816 to be positioned at a plurality of angles relative to the upper housing portion 1804, similar to the screw 1722 in relation to the DRF illustrated and according to various embodiments at 1700.

The upper housing portion 1804, therefore, can define a sidewall 1824 that further defines a bore 1826 so that the screw 1816 can pass therethrough. Further, the lower housing portion 1812 defines a sidewall 1828 and a bore 1830. The bore 1830 defined by the lower housing portion 1802, however, allows for positioning an insert 1832 relative thereto. The insert 1832 can define an upper wall 1834 that defines a portion of a bore 1836. The upper wall 1834 can interact with the polyaxial head 1820 to allow for the screw 1820 to be positioned at an angle relative to a central axis 1838 of the upper housing 1804. The screw 1816 can define a central axis 1840 that can be positioned at an angle 1842 relative to the central axis 1838 of the upper housing 1804. The angle 1842 can be any appropriate angle, for various reasons, including those discussed above, but can be about 0° to 90°.

The insert 1832 can further define a singular projection 1844 or a plurality thereof. The projections 1844 can engage a selected portion of the patient, such as a surface of a bone for various reasons. For example, the projections 1844 can engage the bone to resist rotation of the insert 1832, and therefore, rotation of the DRF 1800. The screw 1816 can provide a force to the upper wall 1834 of the insert into the sidewall 1824 of the upper housing 1804 to assist in resisting rotation of the DRF 1800. Further, because the upper housing 1804 and the lower housing portion 1802 can be interconnected the rotation of the DRF 1800 can be substantially reduced or eliminated.

Further, the insert 1832 can be formed as a separate member or as a single member with the lower housing portion 1802. If the insert 1832 is provided as a separate member, it can be selected either intraoperatively or preoperatively for various purposes. For example, the size, the number, the geometry or the like of the projections 1844 can be selected. Further, the overall size of the insert 1832 can also be selected. The selection of the insert 1832 can be provided for various reasons, such as positioning of the DRF 1800, the size of the patient 14, or other reasons. Regardless,

the insert 1832 can allow for intraoperative selection and specification of the DRF 1800 for various purposes.

The DRF 1800 can be positioned relative to the patient according to any appropriate procedure. For example, as according to various embodiments, a tool 1850 can engage the tool engaging portion 1822 of the screw and be held relative thereto for various reasons. The DRF 1800, either as an assembly or separately, can then be passed through a cannula, an incision, or the like to be positioned relative to the patient 14.

The DRF 1800 can be positioned relative to any portion of the anatomy, including those described above. The DRF 1800 can be positioned relative to a pelvis, an iliac crest of a pelvis, a femur, a tibia, a humerus, a vertebra, or the like. The DRF 1800, however, can include a geometry of the housing portions 1804, 1802 for various purposes, such as subcutaneous movements, percutaneous placements, reduction of interaction with the soft tissue, or any other appropriate reason.

The DRF 1800 can include a dimension 1852 that is defined by a top 1805 of the upper housing portion 1804 and a bottom 1803 of the lower housing portion 1802. The dimension 1852 can be any appropriate dimension, such as those described above, and for example, about 1 mm to about 50 mm. Regardless, the DRF 1800 can include any appropriate dimension for various purposes, including a selected position on the anatomy, a size of a patient, or the like. Also, the DRF 1800, according to various embodiments discussed herein, can include a dimension 1851 that is a dimension that can define a width or diameter of the DRF 1800. The dimension 1851 can be any appropriate size, such as about 1 mm to about 50 mm. The dimension 1851 can also assist with percutaneous and/or subcutaneous positioning and or movement of the DRF 1800.

The DRF 1800 can be formed of any appropriate materials. For example, various polymers, metals, metal alloys, and the like can be selected. The housing portion 1802, 1804 can be formed of a selected material, such that it can deform or conform to a selected portion of the anatomy. For example, the housing portion 1802 can be formed to conform to a portion of the anatomy, such that the anatomy, including a bone surface, need not be substantially flattened or position the DRF 1800 relative thereto. Further, the screw 1816, can be formed of a resorbable material, such that the housing 1802, 1804 can be broken away from the screw 1816 for ease of removal of the housing 1802, 1804 at the screw 1860 will resorb at a selected rate.

It will be understood, that various embodiments of the various DRFs described above. It will be understood, however, that the various adaptations can be formed and still be within the scope of various embodiments and the teachings herein. For example, any appropriate anchor portion can be used to anchor the DRF according to various embodiments relative to the patient 14. For example, a staple, a pin, a rivet, or the like can be used to fix the DRF relative to the anatomy. Further, the DRF can be anchored for anti-rotation or other purposes using portions other than projections extending from a portion of the DRF. For example, an auxiliary pin, screw, rivet, or the like can be positioned through the DRF to assist in reducing or resisting rotation of the DRF relative to the patient 14.

With particular reference to FIG. 84, the DRF 1800, or any DRF according to various embodiments can be positioned in a patient 14 through soft tissue 14a (e.g. skin, dermis, muscle, adipose tissue, or the like) and positioned relative to a bone 14b, such as a femur. As discussed above

the bone **14b** can be prepared or unprepared as selected by a user or the various embodiments.

The incision **1852** can be any appropriate incision and include any appropriate dimension. Generally the dimension of the incision **1852** need not be much greater than any dimension of the DRF **1800**. Such an incision can allow for a percutaneous positioning of the DRF **1800**. Further, the soft tissue **14a** can remain above the DRF **1800**, cover, or re-encapsulate the DRF **1800** after the DRF **1800** is positioned on the bone **14b**. This can allow the bone **14b** to move relative to the soft tissue **14a**, or vice versa, without much interaction or disturbance of the soft tissue **14a**.

Also, the poly-axial anchor **1816** can be positioned at an angle relative to the housing or body **1804**, **1806**. The angle can allow the DRF **1800**, according to various embodiments, to be fixed to the bone **14b** without engaging a portion thereof, such as the intramedullary canal **14c**. The attachment portions, such as the projections **1844**, however, can engage the bone **14b** to assist in resisting rotation of the DRF **1800**, fixation of the DRF **1800** or other appropriate purposes. Also, as discussed herein, the bone **14b** can remain substantially unprepared or natural, if selected, and the DRF can still be mounted thereto.

Initially, it will be understood although various embodiments are not necessarily illustrated to include each of the discussed portions, such as protective sleeves and the like, that each will be available and can be included with the various embodiments. Further, the protective elements, such as the crushable or moving member, can be used to protect various portions. For example the protective elements can protect the patient or the anatomy of the patient into which they are placed. Also, the protective elements can protect the user or the person placing the DRF as the sharp portion is generally covered or not substantially revealed until it engages the bone of the patient. Therefore, it will be understood that the protective element can protect many portions, be it the patient, user, instrument, or any appropriate portion or person.

As discussed above, the DRF, according to various embodiments, can be attached to any selected portion of the anatomy or multiple DRFs can be attached to a plurality of anatomic portions or regions. Also, the DRF according to the various embodiments can be used for any appropriate use. For example, a first DRF can be positioned on a first bone and a second DRF can be positioned on a second bone for determining a position of the DRFs, and therefore the bones, relative to one another. For example, as illustrated above, a first DRF can be positioned on a selected portion of a femur and a second DRF can be positioned on a portion of a pelvis.

Various DRFs can also be positioned on various portions of a single bone or what naturally was a single bone. For example, during a fracture, a single bone may be divided into more than one piece. The fracture may either be complete or partial, but the various portions of the bone may move relative to one another in a non-rigid manner. Therefore, a first DRF and a second DRF can be attached to a first portion of the bone and a second portion of the bone, respectively, to determine a position of the various portions of the bone relative to one another. This can assist in tracking the bone portions to assist in setting bones, positioning various portions of a fractured bone relative to one another and for various other purposes. It will be understood, however, that the various uses described herein are merely exemplary and not intended to limit the scope of the present teachings.

Instruments can be moved relative to the patient **14** and the tracking devices on the instrument can be used to

illustrate the position of the instrument on a display device. The display device can also display image data that is registered to the patient space. The various DRFs can be used to maintain registration even if the patient **14** moves. Alternatively, the patient **14** can be fixed in space during a procedure, thus not requiring any DRFs.

An instrument **1900** is illustrated in FIG. **85**. The instrument **1900** can be any appropriate instrument including those discussed and illustrated above. For example, instrument **1900** can be the stylet portion **156**, suction device **190**, probe device **166**, or any other appropriate instruments. The instrument **1900** can also include other instruments including cranial stylets, biopsy needles, ear nose and throat instruments (e.g. drill guides, shavers, etc.), small diameter dynamic reference frames, transvenous catheters, other catheters, dynamic reference frames or other patient attached devices, and other selected devices. Generally, the selected instrument **1900** can include a long thin configuration, such as that of the stylet **150**. It will be understood, however, that the instrument **1900** can be any appropriate instrument and discussion herein of the stylet **1900** is merely exemplarily.

The instrument **1900**, as the stylet **1900**, can be positioned in selected instruments or can be incorporated with selected instruments. The stylet **1900**, if positioned in another secondary instrument, can be rotationally fixed relative to the secondary instrument along a longitudinal axis. The position of the stylet **1900** can be determined by tracking the location of a tracking device **1910**. The tracking device can include multiple windings or turns of a wire **1912** into a coil, to form the tracking device **1910**. The tracking device **1910** can be wrapped around a long axis **1914** of the instrument **1900**. The tracking device **1910** can include a long axis that is substantially co-axial with the long axis **1914** of the instrument **1900**. It will be further understood, that multiple coils can be used to define a single tracking device, thus each tracking device can be used to identify more than one navigation vector, as discussed herein. Thus, discussion of the tracking device as including only a single coil is for illustration and ease of discussion only.

The long axis **1914** of the instrument **1900** is illustrated in FIG. **85** as being parallel to a line **19141** that is external to the instrument **1900** for illustration purposes of the following discussion. It will be understood that because the long axis **1914** and the line **19141** are parallel that any angle relative to the line **19141** is identical to an angle relative to the long axis **1914** of the instrument **1900**. The windings of the wire **1912** can be wound at an angle **1920** relative to the line **19141**. The angle **1920** can be defined as an angle between the line **19141** and a line that is defined by one of the windings of the wire **1912** or a plane generally through the instrument **1900** defined by a single winding of the wire **1912**. For illustration, the line **1922** can define a line or plane extending from one of the windings of the wire **1912**. As illustrated in FIG. **85**, the angle **1920** is generally non-perpendicular to the line **19141**. The angle **1920** is an acute angle relative to the line **19141**. A supplementary angle will be formed on the reverse side of the line **1922** relative to the line **19141**.

The angle **1920** can be selected in a range of about 10 degrees to about less than 90 degrees, including about 40 degrees to about 50 degrees, and including about 45 degrees. The angle **1920** can be referred to as a winding or coil angle. As discussed herein the winding angle is an angle of the windings of the various coils relative to the long axis around which the coils are wound which can also be a long axis of an instrument around which the coil is wound. The winding angle is substantially an angle that is greater than an angle

formed when a wire is wound tightly in a single layer on an instrument, which can generally form a helix due to the thickness of the wire being wound. The winding angle can be defined relative to the long axis of the coil by two points 5 opposed to one another one a single turn or by a plane through a single turn, as illustrated in FIG. 85.

The tracking device 1910 can be part of an electromagnetic tracking system, as discussed above. In such a system, the wire 1912 can be acted upon by an electromagnetic field or can generate an electromagnetic field. In the example 10 discussed herein, the wire 1912 of the tracking device 1910 can be acted upon by an external magnetic field to generate a current in the wire 1912 or set up the voltage within the wire 1912 of the tracking device 1910.

Because the wire 1912 of the tracking device 1910 is 15 wound at the angle 1920 to the line 19141, a navigation vector 1930 is defined through the tracking device 1910 at an angle 1932. The navigation vector 1930 is generated and based on the tracking system localizer 600. In other words, the angle of the windings 1920 is based on the physical turns of the wire 1912, but the navigation vector 1930 is based on the induced voltage from the localizer 600 and is generally perpendicular to the coils of the wire 1912,1942. The voltage 20 induced in the wire 1912 is proportional to the strength of the magnetic field generated by the localizer 600 multiplied by the cosine of the angle between the vector magnetic field and a line or vector normal to a winding of the wire 1912. Thus, when all other variables of location are known, such as position in space and a field strength of the magnetic field 25 generated by the localizer 600, the angle (e.g. the navigation vector 1930) between the coil's normal and the vector magnetic field can be determined. The determination can be performed by executing instructions with a processor. In other words, the navigation vector can be computed by comparing the measured strength of the magnetic field to the theoretical value at a specific location. It will also be understood that the tracking devices discussed herein can generate a field that is sensed by the localizer for navigation purposes.

The angle 1932 when added to the angle 1920, as illustrated in FIG. 85, can equal substantially 180 degrees. Accordingly, the angle of the navigation vector 1932 and the angle of the coil winding 1920 can be substantially supplementary angles.

The external field that can induce a current in the wire 45 1912 due to generally understood and accepted electromagnetic properties. Accordingly, the operation of the tracking device 1910 will not be discussed in detail here, however, it is discussed above. The position of the navigation vector 1930 can be used to identify the location of the instrument 1900 and to determine the orientation of the tracking device 1910 in space (e.g. patient space). The orientation of the navigation vector 1930 relative to the long axis 1940 of the instrument allows for multiple tracking devices to be positioned on the instrument including navigation vectors that are all non-perpendicular to the long axis 1914 of the instrument 1900. For example, a second tracking device 1940 can include a wire 1942 that is wound around the instrument 1900 to form a coil that has a coil axis 1944 at an angle 1946 relative to the line 19141. The second tracking device 1940 therefore defines a navigation vector 1950 that has a second navigation vector angle 1952. The second navigation vector angle 1952 is also supplementary to the angle 1946 of the tracking device 1940. The navigation vector angle 1932 of the first tracking device 1910 can be 65 different than the navigation vector angle 1952 of the second tracking device. With the two tracking devices 1910, 1940

six-degree of freedom information (6DOF), including x, y, and z positions and three degree of orientation can be determined. Though more than two tracking devices can be included, they are not necessary to determine the 6DOF location information regarding the instrument 1900.

As illustrated in FIGS. 86A and 86B, the vectors 1930, 1950 can provide orientation information regarding the two tracking devices 1910, 1940 positioned on the instrument 1900 relative to a coordinate system 1960. The coordinate system 1960 can be a three dimensional coordinate system 10 having three orthogonal axes 1960x, 1960y, and 1960z. Within the coordinate system 1960 the vectors 1930, 1950 can be used to identify locations of the tracking devices 1910, 1940 in the three dimensional coordinate system 1960. The navigation system can be used to determine the location information by executing instructions based on the signal received about the tracking devices 1910, 1940. 15

The vectors 1930, 1950 regarding the orientation of the respective tracking devices 1910, 1940 relative to the centers 20 1910c, 1940c can be used to determine location information, including position and orientation information, regarding the two tracking devices 1910, 1940. Although the single position and orientation information for any one of the tracking devices 1910, 1940 may not be enough information to identify all location information for the instrument 1900, the information regarding both of the tracking devices 1910, 1940 can be used to identify six degree of freedom information regarding the instrument 1900. 25

The vectors 1930, 1950 both extend through respective centers 30 1910c, 1940c of the respective tracking devices 1910, 1940. Accordingly, the direction of the vectors 1930, 1950 in combination with the three dimensional coordinate positions of the center of the respective tracking devices 1910c, 1940c can be used to identify the location information of the instrument 1900. As illustrated in FIGS. 86A and 86B as the instrument 1900 is rotated in space the vectors will change direction. Because the vectors are non-normal to the instrument 1900 a rotation of the instrument 1900 can be efficiently determined, including the amount of rotation and orientation in all three of roll, pitch, and yaw. As illustrated between FIGS. 86A and 86B the orientation of the two vectors 1930, 1950 are substantially different relative to the long axis 1914 of the instrument 1900. Again, location information includes both x, y, and z axis position information and roll, pitch, and yaw orientation. 45

With reference to FIGS. 87A and 87B, an instrument 1970, which can be similar to the instrument 1900, can include at least three tracking devices 1972w, 1974w, and 1976w. Each of the tracking devices can be formed around the instrument 1970 similar to the tracking devices 1910, 1940 discussed above. Each of the tracking devices 1972w, 1974w, and 1976w positioned on the instrument 1970 can include a navigation vector 1972, 1974, 1976. Therefore, a first navigation vector 1972 can be formed by a first tracking device 1972w, a second navigation vector 1974 can be formed by a second tracking device 1974w, and a third navigation vector 1976 can be formed by a third tracking device 1976w relative to the instrument 1970. Each of the navigation vectors 1972-1976 can be formed relative to the instrument 1970 due to the positioning of the windings of material of the respective tracking devices 1972w, 1974w, and 1976w at the winding angle relative to the instrument 1970. 50

FIG. 87A attempts to illustrate on a two-dimensional plane of a page a three-dimensional rotation of angles of the three different windings 1972w, 1974w, and 1976w. As discussed above, in relation to FIG. 85, each of the windings 65

can be wound at the winding angle relative to a long axis **1914** of the instrument **1900**. As illustrated in FIGS. **87A** and **87B**, however, rather than having the windings formed at various and different winding angles relative to the long axis **1980** of the instrument **1970** (as the windings are illustrated in FIG. **85**), each of the windings can be formed at substantially a single winding angle, including those winding angles discussed above and such as about 20 degrees to about 70 degrees, relative to the long axis **1980** of the instrument **1970**.

Because each of the coils of the tracking device windings **1972_w**, **1974_w**, and **1976_w** are at the same winding angle, to resolve the six degrees of freedom a top **1972_{wt}**, **1974_{wt}**, and **1976_{wt}** of each of the coil windings **1972_w**, **1974_w**, and **1976_w** are rotated a rotation angle, such as about 120 degrees relative to one another around the long axis **1980** of the instrument **1970**. As discussed above, however, three windings are not required and an appropriate number of windings can be used with an appropriate number of localizer coils. The rotation angle RA can be selected to be 120 degrees to place each of the tops **1972_{wt}**, **1974_{wt}**, **1976_{wt}** substantially equidistant apart around the long and central axis **1980** of the instrument **1970**. It will be understood, however, that the rotation angle RA can be about 90 degrees to about 180 degrees, including about 120 degrees. Also, a rotational distance between each top or winding **1972_w**-**1976_w** can be different, such as RA₁, RA₂, and RA₃.

As illustrated in FIG. **87B**, the front or top end of the windings **1972_{wt}**-**1976_{wt}** are all in substantially the same direction, such as towards a distal end of the instrument **1970**. Each of the windings **1972_w**-**1976_w** rotationally spaced apart around the center long axis **1980** of the instrument **1970**. In this way, the navigation vectors **1972-1976** for each of the windings **1972_w**-**1976_w** can be formed at the same winding angle relative to the long axis **1980** of the instrument **1970**. The navigation vectors **1972-1976** are also, due to the rotational spacing of the coil windings tops **1972_{wt}**-**1976_{wt}**, rotationally spaced around the long axis **1980**.

The different navigation vectors **1972-1976** are defined relative to a center **1980** of the instrument **1970**. Each of the vectors **1972-1976** can point towards a plane P, as illustrated in FIG. **87A**, which can be illustrated in FIG. **87B** as the plane of the page. The tails of the vectors **1972-1976** can go into and past the plane on the page illustrating FIG. **87B**, thus all of the navigation vectors **1972-1976** are not coplanar, but they all intersect the single plane P. Each of the vectors **1972-1976** can be formed relative to the plane P rotationally spaced at the RA angle relative to one another around the center **1980** of the instrument **1970**.

As discussed above, the navigation vector angle can be selected by forming the windings of the tracking device **1972_w**-**1976_w** at a selected angle relative to the long axis of the coil winding **1972_w**-**1976_w**. By changing the positioning of the angle of the rotation of the windings of the various tracking devices, the navigation vectors can be positioned relative to the instrument **1970** in this selected manner. In various embodiments, the vectors **1972-1976** are differently oriented relative to the instrument **1980** by having more than one coil wound at the same winding angle, but being spaced relative to one another with the RA angle.

Accordingly, not only can navigation vectors include supplementary angles relative to the long axis of the instrument **1900**, as illustrated by the navigation vector angle **1932**, **1952**, they can also be formed to be at a selected angle relative to a long axis of the instrument **1970**, but positioned around the center of the instrument **1980** to have an angle of

about 120 degrees to one another. The RA angle between the navigation vectors **1972-1976**, however, can be at a selected angle, such as an angle between about 10 degrees to about 180 degrees, including about 90 to about 180 degrees, further including about 120 degrees. It will be further understood that each tracking device that defines the respective navigation vectors **1972-1976** can be formed or defined by tracking devices that are non-overlaid or are sequential along the instrument **1970**. Although tracking devices can be positioned sequentially, or non-overlaid on an instrument, tracking devices can be overlaid, as illustrated in FIG. **88**, on an instrument **1990**. The instrument **1990** can include a first tracking device **1992** and a second tracking device **1994**. The instrument **1990** can include or define a long axis **1996** that is illustrated parallel to a line **19961**. As discussed above, the line **19961** is drawn for illustration in FIG. **88** of the current discussion. When overlaid a layer of insulation, either on the wire, between the windings, or both, can be provided between the two tracking portions **1992** and **1994**. Also, three or more windings can also be provided.

A first tracking device **1992** can be formed with a first wire winding **1998** similar to the wire **1912** of the first tracking device **1910**. The tracking device **1992**, having the wire winding **1998**, can define a winding axis **2000** that is at an angle **2002** relative to the line **19961**. The first tracking device **1992** can therefore define a navigation vector **2004** that is at an angle **2006** relative to the line **19961**. As discussed above, the angle **2002** and **2006** can be supplementary to each other relative to the line **19961**. In a similar manner, a second tracking device **1994** can include a wire winding **2008** that can define a wire winding axis **2010** having an angle **2011** and a navigation vector **2012** having an angle **2013**.

The two tracking devices **1992**, **1994** can be similar to the two tracking devices **1910**, **1940** discussed above. The navigation vectors **2004**, **2012** can be at similar angles to the line **1996** as the navigation vectors **1930**, **1950** to the line **19141**. The two tracking devices **1992**, **1994**, however, can be formed over each other, also referred to as overlaid, on the instrument **1990**. Overlaying the two tracking devices **1992**, **1994** on one another can be provided to substantially eliminate a possibility of movement between the two tracking devices. However, even if the wire **1998**, **2008** of the two tracking devices **1992**, **1994** is thin or has a small diameter, the diameter at the tracking devices **1992**, **1994** of the wire is doubled by overlaying them. Accordingly, having sequential tracking devices, such as the first and second tracking devices **1910**, **1940** on the instrument **1900** illustrated in FIG. **85**, can be provided to minimize the diameter of the instrument and tracking devices. Each of the tracking devices **1992**, **1994** can be insulated from one another and from the instrument **1900** with insulation. The insulation can be a shrink wrap, insulated wire for the windings, or other selected insulation portions.

The two tracking devices **1992**, **1994**, however, can still define multiple navigation vectors relative to a single tracking device center point **2020_c**. As illustrated in FIGS. **89A** and **89B**, the navigation vectors **2004**, **2012** can both extend through the single center point **2020_c** in the coordinate system **1960**. Again, the plurality of the navigation vectors **2004**, **2012** that do not extend at an identical angle from the long axis **1996** of the instrument **1990** can allow for determination of an orientation and a position of the instrument **1990** with six degrees of freedom.

With reference to FIG. **90**, and drawing on the description of the stylet **150** above, a stylet **150'** is illustrated. The stylet **150'** can include portions substantially similar or identical to

the portions discussed above, with like reference numerals augmented with a prime in FIG. 90. The stylet 150', however, can include tracking devices such as the tracking devices 1910, 1940 along the length of the stylet 150'. The various tracking devices along the stylet 150' can provide navigation vectors in a plurality of orientations relative to the long axis 1501 of the stylet 150'. Navigation vectors can include a first navigation vector 2030, a second navigation vector 2032, and a third navigation vector 2034. The first navigation vector 2030 can be on the plane of the page and form an angle and be pointed towards a proximal end of the stylet 150'. The second navigation vector 2032 can be substantially parallel to the plane of the page and be pointed towards the distal end of the stylet 150'. The third navigation vector 2034 can extend out of the plane of the page and also have an angle towards the proximal end of the stylet 150'.

The various navigation devices can also be positioned on or with other instruments, such as a biopsy needle 2040, illustrated in FIGS. 91A and 91B. A biopsy needle can include an appropriate biopsy needle such as the biopsy needle sold by Medtronic Navigation, Inc. and generally understood in the art. Briefly, the biopsy needle 2040 can include a resection or biopsy port 2042. As is understood by one skilled in the art, a biopsy port 2042 allows for tissue to be drawn in the biopsy needle 2042 for testing and various biopsy procedures.

By positioning the tracking devices on the biopsy needle 2040, a plurality of navigation vectors 2044, 2046, and 2048 can be used to identify the location of the biopsy needle port 2042 on the display device 2034. The location information, again, can include six degrees of freedom information. Thus, complete three-dimensional location information regarding the resection port 2042 can be determined. In knowing the location of the biopsy port 2042, the user 614 can be ensured that the appropriate tissue is being biopsied from within the patient 14.

With reference to FIG. 91B, the display 34 can illustrate image data 36 of the patient 14. The image data 36 can include information, such as of a portion of the patient 14 to be resected 2049. Icons can be displayed on the display device 34 representing the instrument 2040 with an instrument icon 2040'. As discussed above, a window, such as a biopsy window 2042 can be formed in the instrument 2040. The biopsy window 2042 generally includes only a selected cone of resection into which material can be drawn for biopsy. Accordingly, the direction of the cone can be displayed on the display device 34 with a biopsy cone icon 2042'. Because the cone generally extends at only a single angle relative to the instrument 2040, knowing six degrees of freedom information regarding the location of the biopsy window 2042 can assist the user 614 by illustrating the location of the biopsy cone 2042' on the display 34. In this way, the user 614 can view and confirm that the resection cone is aimed or at the tissue to be resected.

In a further example, as illustrated in FIG. 92, an instrument 2050 can be positioned in a heart 2052 of the patient 14. The instrument 2050 can include an ablation or sensing portion 2054 that is positioned at a selected location on the instrument 2050. Again, by providing the plurality of tracking devices on the instrument 2050, the three-dimension location of the ablation portion 2054 can be determined and illustrated on the display device 34 relative to the image data. Alternatively, only the location can be illustrated without reference to other image data just for reference of the location of the instrument 2050. Accordingly, the user

614 can understand the orientation of the instrument 2050 for ensuring an appropriate location of the ablation portion 2054 within the heart 2052.

It is understood that image data and icons representing instruments can be displayed on the display device 34, thus FIG. 92 can be understood to represent image data and icons on the display device 34. The catheter or instrument 2050 can be used to guide a needle or other instrument, such as an ablation needle 2056, through the catheter 2050. The ablation needle 2056 can include an ablation end 2058 which extends through an opening 2060 in the catheter 2050. The opening 2060 in the catheter 2050 can be a single opening, similar to the biopsy window 2042 of the biopsy instrument 2040. The opening 2060 can extend or allow the needle 2058 to extend substantially in only a single direction or position from the catheter 2050. Accordingly, again knowing six degree of freedom information regarding the location of the opening 2060, can assist the user in understanding the location of the ablation portion 2058 within the patient 14. It will be understood that image data of the heart 2052 can be displayed on the display device 34 as can icons representing the location of the various portions, including the ablation needle 2056, the ablation portion 2058, and the opening 2060.

The various tracking devices, as discussed above, can be positioned at a plurality of locations along an instrument, such as an instrument 2070, as illustrated in FIG. 93A. The instrument 2070 can be a selected instrument that has a length and may be flexible or moveable along its length, such as the instrument 2050 illustrated in FIG. 92 including a catheter, ablation probes, or the like. The instrument 2070 can be moved through the patient 14 or any other appropriate subject and can achieve multiple configurations and orientations based upon a movement, either intended or unintended. Therefore, the instrument 2070 can move to a second orientation or location 2070', as illustrated in FIG. 93B.

Positioned along the instrument can be a plurality of tracking devices including a first tracking device 2072, a second tracking device 2074, a third tracking device 2076, and a fourth tracking device 2078. The tracking devices can include the tracking devices discussed above including the first winding 1912 and the second winding 1942. It will be understood that a number of windings or portions can be included for each of the tracking devices and that groups of windings, including three windings, can be used to form each of the tracking devices 2072-2078. As illustrated in FIG. 87, each of the tracking device portions can include a navigation vector that is angled relative to one another, which can allow for the determination of six degrees of freedom. Accordingly, each tracking device can be formed by a plurality of windings that form a tracking device coil having a navigation vector defined through each of the windings.

By providing a plurality of tracking devices 2072-2078 on the single instrument 2070, a location and a relative orientation vector 2072_v-2078_v can be determined at each of the locations of the tracking devices 2072-2078. The location can be determined with the tracking system. Also, the relative orientation of the various tracking devices 2072-2078, relative to the others or to an initial orientation, can be illustrated. This can allow for a substantially discreet and complex view of a location of different portions of the instrument 2070 within the patient 14.

As illustrated in FIG. 93A, each of the relative orientation vectors 2072_v-2078_v point generally towards one side of the instrument 2070. It will be understood that the relative orientation vectors 2072_v-2078_v can relate to a determined

orientation based upon the individual navigation vectors of the portions of the tracking devices **2072-2078**. Accordingly, it will be understood that each of the tracking devices **2072-2078** can each include a plurality of navigation vectors and the relative orientation vector **2072v-2078v** is based upon the determination of each of the plurality of navigation vectors.

At a selected time, which can be after the time for which the location information is determined and illustrated in FIG. **93A**, the instrument can change to a different configuration as illustrated as instrument **2070'** illustrated in FIG. **93B**. The instrument **2070'** still includes each of the tracking devices **2072-2078** and each of the tracking devices can include a relative orientation vector **2072V-2078V**. Each of the relative orientation vectors **2070v'-2078v'** can be used to determine a new or different location of the instrument **2070** and this information can be used to determine if the instrument **2070** has moved to a selected configuration or has moved from a selected configuration to an unselected configuration. Regardless, the plurality of tracking devices can be provided to determine detailed information for the user **614** regarding the location information for several portions of the instrument **2070**.

The teachings herein are merely exemplary in nature and, thus, variations that do not depart from the gist of the teachings are intended to be within the scope of the teachings. Such variations are not to be regarded as a departure from the spirit and scope of the teachings.

What is claimed is:

- 1.** A trackable instrument assembly, comprising:
an elongated guide defining a first bore extending from a first proximal end to a first distal end;
an elongated sleeve defining a second bore extending from a second proximal end to a second distal end, the elongated sleeve sized and configured to be slidably inserted in the first proximal end of the elongated guide and positionable in the first bore of the elongated guide;
at least one tracking device attached to the elongated sleeve; and
a tool extending from a third proximal end to a third distal end, the tool sized and configured to be slidably inserted in the second proximal end of the elongated sleeve and positionable and rotatable in the second bore of the elongated sleeve while the elongated sleeve is positioned in the first bore of the elongated guide;
wherein the at least one tracking device is configured to be used to track a selected portion of the tool.
- 2.** The trackable instrument assembly of claim **1**, wherein the at least one tracking device is attached about the second bore at the second distal end of the elongated sleeve, wherein the tool is positioned in the second bore and adjacent the at least one tracking device.
- 3.** The trackable instrument assembly of claim **2**, wherein the selected portion of the tool is the third distal end of the tool.
- 4.** The trackable instrument assembly of claim **3**, wherein the tool is a drill bit having a drill tip at the third distal end.
- 5.** The trackable instrument assembly of claim **4**, wherein the drill bit includes a stop member for interacting with the second proximal end of the elongated sleeve as the drill tip extends beyond the first distal end of the elongated guide.
- 6.** The trackable instrument assembly of claim **4**, wherein the drill bit includes a tool engaging portion at the third proximal end wherein the drill bit is configured to rotate relative to the elongated sleeve.

7. The trackable instrument assembly of claim **1**, further comprising a spring configured to be positionable in the first bore and about the tool to assist in tracking a selected portion of the tool.

8. The trackable instrument assembly of claim **7**, wherein the spring is configured to be compressed a selected distance during movement of the tool.

9. The trackable instrument assembly of claim **1**, wherein the elongated guide further includes a handle.

10. The trackable instrument assembly of claim **1**, wherein the at least one tracking device is a tracking coil positioned relative to the second distal end of the elongated sleeve.

11. The trackable instrument assembly of claim **1**, wherein the at least one tracking device includes a first tracking device and a second tracking device.

12. The trackable instrument assembly of claim **1**, wherein the tool is selected from a drill bit or an awl.

13. The trackable instrument assembly of claim **1**, wherein the trackable instrument assembly is formed of a substantially non-magnetic material.

14. The trackable instrument assembly of claim **1**, wherein the elongated guide defines an elongated slot configured to accommodate a connection to the at least one tracking device.

15. A trackable instrument assembly, comprising:
a first tube having a handle and defining a first bore extending from a first proximal end to a first distal end;
a second tube defining a second bore extending from a second proximal end to a second distal end, the second tube sized and configured to be slidably inserted in the first proximal end of the first tube and movably positionable within the first bore of the first tube;
at least one tracking sensor attached to the second distal end of the second tube; and
a drill bit extending from a tool engaging proximal end to a drill bit tip distal end, the drill bit sized and configured to be slidably inserted in the second proximal end of the second tube and rotated and positioned within the second bore of the second tube while the second tube is positioned in the first bore of the first tube;
wherein the at least one tracking sensor is configured to track the drill bit tip distal end of the drill bit.

16. The trackable instrument assembly of claim **15**, wherein the at least one tracking sensor is a tracking coil wrapped around the second distal end of the second tube so that the second bore is open to receive the drill bit there-through.

17. The trackable instrument assembly of claim **15**, wherein the at least one tracking sensor includes two spaced-apart tracking sensors positioned on the second tube such that the distance and orientation between the two tracking sensors remains substantially constant.

18. The trackable instrument assembly of claim **15**, further comprising a spring configured to be positionable in the first bore and about the drill bit to assist in tracking the drill bit.

19. A trackable instrument assembly, comprising:
an external tube having a handle and defining a cannula extending from a first proximal tube end of the external tube to a second distal tube end of the external tube;
a sleeve defining a sleeve bore extending from a first proximal sleeve end to a second distal sleeve end, the sleeve sized and configured to be slidably inserted in the first proximal tube end and moveably positioned in the cannula of the external tube;

99**100**

at least one tracking sensor attached to the second distal sleeve end of the sleeve; and

a tool extending from a first proximal tool end to a second distal tool end, the tool sized and configured to be slidably inserted in the first proximal sleeve end and 5 movable and rotatable in the sleeve bore of the sleeve while the sleeve is positioned in the cannula of the external tube;

wherein the at least one tracking sensor is configured to track a selected portion of the tool. 10

20. The trackable instrument assembly of claim **19**, wherein the at least one tracking sensor is operated either substantially wired or wireless.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 11,331,150 B2
APPLICATION NO. : 15/362094
DATED : May 17, 2022
INVENTOR(S) : Bradley A. Jascob et al.

Page 1 of 4

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

Item (56) Column 2, Line 1, delete “Electromagetic” and insert --Electromagnetic-- therefor

Page 7, Item (56) Column 1, Line 16, delete “”Three-Dimensinal” and insert --“Three-Dimensional--
therefor

Page 7, Item (56) Column 1, Line 35, delete “localizationusing” and insert --localization using--
therefor

Page 7, Item (56) Column 2, Line 7, delete “RoboticsandComputer-Assisted” and insert --Robotics
and Computer-Assisted-- therefor

Page 8, Item (56) Column 1, Line 29, delete “Tomograhic” and insert --Tomographic-- therefor

Page 8, Item (56) Column 1, Line 30, delete “Fluorscopic” and insert --Fluoroscopic-- therefor

Page 8, Item (56) Column 1, Line 50, delete “Millenium,” and insert --Millennium,-- therefor


Page 8, Item (56) Column 2, Line 4, delete “Internatjional Searh” and insert --International Search--
therefor

Page 8, Item (56) Column 2, Line 12, delete “Imgaging” and insert --Imaging-- therefor

In the Specification

Column 17, Line 52, delete “84” and insert --14-- therefor

Column 18, Line 62, delete “78” and insert --76-- therefor

Signed and Sealed this
Ninth Day of August, 2022

Katherine Kelly Vidal
Director of the United States Patent and Trademark Office

Column 19, Line 13, after "98", insert ---

Column 19, Line 62, delete "106" and insert --108-- therefor

Column 24, Line 67, delete "48." and insert --46.-- therefor

Column 39, Line 17, delete "434." and insert --436.-- therefor

Column 39, Line 19, delete "434" and insert --436-- therefor

Column 39, Line 58, delete "464" and insert --462-- therefor

Column 40, Line 31, delete "The" and insert --They-- therefor

Column 43, Line 36, delete "522," and insert --520,-- therefor

Column 48, Line 33, delete "12" and insert --612-- therefor

Column 48, Line 35, delete "12," and insert --612,-- therefor

Column 50, Line 39, delete "filed" and insert --field-- therefor

Column 50, Line 44, delete "filed" and insert --field-- therefor

Column 58, Line 54, delete "800" and insert --808-- therefor

Column 59, Line 37, delete "810" and insert --816-- therefor

Column 60, Line 12, delete "800," and insert --808,-- therefor

Column 62, Line 11, delete "connector" and insert --connector-- therefor

Column 62, Line 51, delete "908," and insert --904,-- therefor

Column 67, Line 3, delete "1022" and insert --1020-- therefor

Column 67, Line 27, delete "1020." and insert --1050.-- therefor

Column 67, Line 46, delete "connector" and insert --connector-- therefor

Column 72, Line 12, delete "1160" and insert --1162-- therefor

Column 72, Line 14, delete "1110" and insert --1100-- therefor

Column 75, Line 25, delete "1212." and insert --1202.-- therefor

Column 76, Line 48, delete “1206” and insert --1202-- therefor

Column 78, Line 33, after “above.”, delete “¶”

Column 79, Line 6, delete “bon” and insert --bone-- therefor

Column 80, Line 22, delete “1424” and insert --1406-- therefor

Column 85, Line 1, delete “1728” and insert --1722-- therefor

Column 87, Line 39, delete “1820” and insert --1816-- therefor

Column 88, Line 48, delete “1860” and insert --1816-- therefor

Column 90, Line 41, delete “19141” and insert --1914l-- therefor

Column 90, Line 44, delete “19141” and insert --1914l-- therefor

Column 90, Line 45, delete “19141” and insert --1914l-- therefor

Column 90, Line 48, delete “19141.” and insert --1914l.-- therefor

Column 90, Line 49, delete “19141” and insert --1914l-- therefor

Column 90, Line 55, delete “19141.” and insert --1914l.-- therefor

Column 90, Line 56, delete “19141.” and insert --1914l.-- therefor

Column 90, Line 58, delete “19141.” and insert --1914l.-- therefor

Column 91, Line 16, delete “19141,” and insert --1914l,-- therefor

Column 91, Line 60, delete “19141.” and insert --1914l.-- therefor

Column 92, Line 1, delete “(6DOF),” and insert --(6 DOF),-- therefor

Column 92, Line 4, delete “6DOF” and insert --6 DOF-- therefor

Column 94, Line 15, delete “19961.” and insert --1996l-- therefor

Column 94, Line 16, delete “19961” and insert --1996l-- therefor

Column 94, Line 25, delete “19961.” and insert --1996l.-- therefor

Column 94, Line 27, delete “19961.” and insert --1996l.-- therefor

CERTIFICATE OF CORRECTION (continued)
U.S. Pat. No. 11,331,150 B2

Column 94, Line 29, delete "19961." and insert --1996l.-- therefor

Column 94, Line 38, delete "19141." and insert --1914l.-- therefor

Column 95, Line 26, delete "2042" and insert --2040-- therefor