

US011389275B2

(12) **United States Patent**  
**Robb et al.**

(10) **Patent No.:** **US 11,389,275 B2**  
(45) **Date of Patent:** **Jul. 19, 2022**

(54) **TEMPORARY ABUTMENT WITH  
COMBINATION OF SCANNING FEATURES  
AND PROVISIONALIZATION FEATURES**

(58) **Field of Classification Search**  
CPC ..... A61C 8/008; A61C 8/005; A61C 8/0068;  
A61C 8/006; A61C 8/0066; A61C  
8/0077;

(71) Applicant: **BIOMET 3I, LLC**, Palm Beach  
Gardens, FL (US)

(Continued)

(72) Inventors: **T. Tait Robb**, Stewart, FL (US);  
**Stephen M. Herrington**, Naples, FL  
(US); **Miguel G. Montero**, Boynton  
Beach, FL (US); **Ralph E Goodman**,  
West Palm Beach, FL (US); **Dan P**  
**Rogers**, Palm Beach Gardens, FL (US);  
**John J. Bellanca**, West Palm Beach,  
FL (US); **Zachary B. Suttin**, West  
Palm Beach, FL (US)

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,732,621 A 5/1973 Bostrom  
3,906,634 A 9/1975 Aspel

(Continued)

FOREIGN PATENT DOCUMENTS

DE 2114323 A1 10/1971  
DE 3531389 A1 3/1987

(Continued)

(\*) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 0 days.

OTHER PUBLICATIONS

“U.S. Appl. No. 13/798,894, Advisory Action dated May 18, 2015”,  
3 pgs.

(Continued)

(21) Appl. No.: **16/445,978**

(22) Filed: **Jun. 19, 2019**

*Primary Examiner* — Jacqueline T Johanas  
*Assistant Examiner* — Shannel Nicole Belk

(65) **Prior Publication Data**

US 2019/0298497 A1 Oct. 3, 2019

**Related U.S. Application Data**

(63) Continuation of application No. 14/575,717, filed on  
Dec. 18, 2014, now Pat. No. 10,368,964, which is a  
(Continued)


(51) **Int. Cl.**  
**A61C 8/00** (2006.01)  
**A61C 13/00** (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **A61C 8/005** (2013.01); **A61C 8/006**  
(2013.01); **A61C 8/008** (2013.01); **A61C**  
**8/0048** (2013.01);  
(Continued)

(57) **ABSTRACT**

A lower region of a temporary abutment includes an anti-rotational feature for non-rotationally mating with a dental implant. An upper region of the temporary abutment includes a first anti-rotational structure and at least one retention groove. A top surface of the temporary abutment includes one or more informational markers that provide information concerning the dental implant. A temporary abutment cap is configured to be coupled to the upper region of the temporary abutment. The temporary abutment cap has at least one projection configured to mate with the at least one retention groove of the temporary abutment. The temporary abutment cap has a second anti-rotational structure that is configured to slidably engage the first anti-rotational structure of the temporary abutment. The temporary abut-

(Continued)

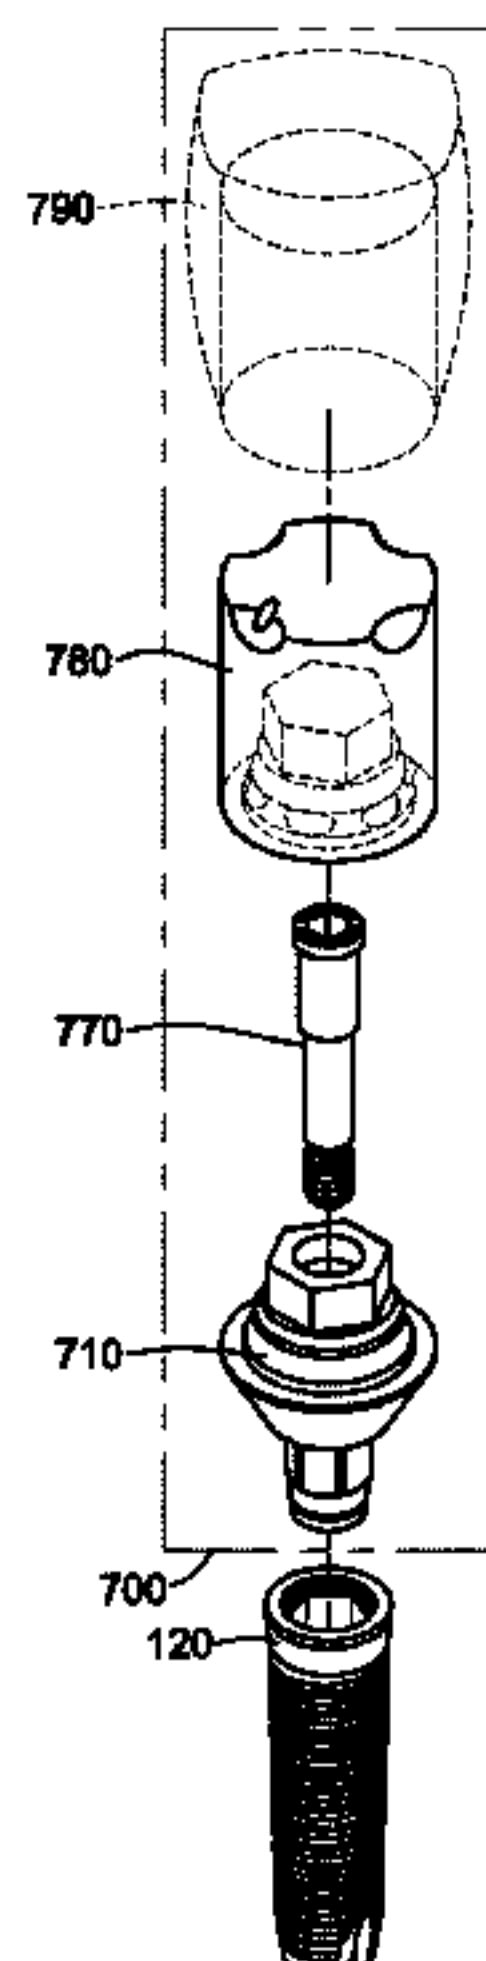

ment cap is configured to be coupled with a temporary prosthesis such that the temporary prosthesis and the temporary abutment cap are removable from the temporary abutment.

### 16 Claims, 31 Drawing Sheets

### Related U.S. Application Data

continuation of application No. 13/473,202, filed on May 16, 2012, now Pat. No. 8,944,816.

(60) Provisional application No. 61/486,630, filed on May 16, 2011.

### (51) Int. Cl.

*A61C 9/00* (2006.01)

*A61C 13/107* (2006.01)

*A61C 13/265* (2006.01)

### (52) U.S. Cl.

CPC ..... *A61C 8/0068* (2013.01); *A61C 9/004* (2013.01); *A61C 13/0001* (2013.01); *A61C 13/0003* (2013.01); *A61C 13/0004* (2013.01); *A61C 8/0001* (2013.01); *A61C 8/0024* (2013.01); *A61C 13/2656* (2013.01); *A61C 2008/0084* (2013.01)

### (58) Field of Classification Search

CPC ..... *A61C 8/0001*; *A61C 13/0001*; *A61C 13/2656*; *A61C 2008/0084*

See application file for complete search history.

### (56) References Cited

#### U.S. PATENT DOCUMENTS

3,919,772 A 11/1975 Lenczycki  
3,958,471 A 5/1976 Muller  
4,011,602 A 3/1977 Rybicki et al.  
4,056,585 A 11/1977 Waltke  
4,086,701 A 5/1978 Kawahara et al.  
4,177,562 A 12/1979 Miller et al.  
4,294,544 A 10/1981 Altschuler et al.  
4,306,862 A 12/1981 Knox  
4,325,373 A 4/1982 Slivenko et al.  
4,341,312 A 7/1982 Scholer  
4,364,381 A 12/1982 Sher  
4,439,152 A 3/1984 Small  
4,543,953 A 10/1985 Slocum et al.  
4,547,157 A 10/1985 Driskell  
4,571,180 A 2/1986 Kulick  
4,611,288 A 9/1986 Duret et al.  
4,615,678 A 10/1986 Moermann et al.  
4,624,673 A 11/1986 Meyer  
4,663,720 A 5/1987 Duret et al.  
4,713,004 A 12/1987 Linkow et al.  
4,756,689 A 7/1988 Lundgren et al.  
4,758,161 A 7/1988 Niznick  
4,767,331 A 8/1988 Hoe  
4,772,204 A 9/1988 Soderberg  
4,793,808 A 12/1988 Kirsch  
4,821,200 A 4/1989 Oberg  
4,842,518 A 6/1989 Linkow et al.  
4,850,870 A \* 7/1989 Lazzara ..... *A61C 8/0048*  
433/174  
4,850,873 A 7/1989 Lazzara et al.  
4,854,872 A 8/1989 Detsch  
4,856,994 A 8/1989 Lazzara et al.  
4,872,839 A 10/1989 Branjnovic  
4,906,191 A 3/1990 Soderberg  
4,906,420 A 3/1990 Branjnovic et al.  
4,931,016 A 6/1990 Sillard

4,935,635 A 6/1990 O'harra  
4,955,811 A 9/1990 Lazzara et al.  
4,961,674 A 10/1990 Wang et al.  
4,964,770 A 10/1990 Steinbichler et al.  
4,986,753 A 1/1991 Sellers  
4,988,297 A 1/1991 Lazzara et al.  
4,988,298 A 1/1991 Lazzara  
4,998,881 A 3/1991 Lauks  
5,000,685 A 3/1991 Branjnovic  
5,006,069 A 4/1991 Lazzara et al.  
5,015,183 A 5/1991 Fenick  
5,015,186 A 5/1991 Detsch  
5,030,096 A 7/1991 Hurson et al.  
5,035,619 A 7/1991 Daftary  
5,040,982 A 8/1991 Stefan-Dogar  
5,040,983 A 8/1991 Binon  
5,064,375 A 11/1991 Jorneus  
5,071,351 A 12/1991 Green, Jr. et al.  
5,073,111 A 12/1991 Daftary  
5,087,200 A 2/1992 Branjovic et al.  
5,100,323 A 3/1992 Friedman et al.  
5,104,318 A 4/1992 Piche  
5,106,300 A 4/1992 Voitik  
5,122,059 A 6/1992 Durr et al.  
5,125,839 A 6/1992 Ingber et al.  
5,125,841 A 6/1992 Carlsson et al.  
5,133,660 A 7/1992 Fenick  
5,135,395 A 8/1992 Marlin  
5,145,371 A 9/1992 Jorneus  
5,145,372 A 9/1992 Daftary et al.  
5,176,516 A 1/1993 Koizumi  
5,188,800 A 2/1993 Green et al.  
5,195,892 A 3/1993 Gersberg  
5,205,745 A 4/1993 Kamiya et al.  
5,209,659 A 5/1993 Friedman et al.  
5,209,666 A 5/1993 Balfour et al.  
5,213,502 A 5/1993 Daftary  
5,221,204 A 6/1993 Kruger et al.  
5,237,998 A 8/1993 Duret et al.  
5,246,370 A 9/1993 Coatoam  
5,257,184 A 10/1993 Mushabac  
5,281,140 A 1/1994 Niznick  
5,286,195 A 2/1994 Clostermann  
5,286,196 A 2/1994 Branjovic et al.  
5,292,252 A 3/1994 Nickerson et al.  
5,297,963 A 3/1994 Daftary  
5,302,125 A 4/1994 Kownacki et al.  
5,312,254 A 5/1994 Rosenlicht  
5,312,409 A 5/1994 McLaughlin et al.  
5,316,476 A 5/1994 Krauser  
5,320,529 A 6/1994 Pompa  
5,322,436 A 6/1994 Horng et al.  
5,328,371 A 7/1994 Hund et al.  
5,334,024 A 8/1994 Niznick  
5,336,090 A 8/1994 Wilson et al.  
5,338,196 A 8/1994 Beaty et al.  
5,338,198 A 8/1994 Wu et al.  
5,343,391 A 8/1994 Mushabac  
5,344,457 A 9/1994 Pilliar et al.  
5,350,297 A 9/1994 Cohen  
5,359,511 A 10/1994 Schroeder et al.  
5,362,234 A 11/1994 Salazar et al.  
5,362,235 A 11/1994 Daftary  
5,368,483 A 11/1994 Sutter  
5,370,692 A 12/1994 Fink et al.  
5,372,502 A 12/1994 Massen et al.  
5,386,292 A 1/1995 Massen et al.  
5,401,170 A 3/1995 Nonomura  
5,413,481 A 5/1995 Goppel et al.  
5,417,569 A 5/1995 Perisse  
5,417,570 A 5/1995 Zuest et al.  
5,419,702 A 5/1995 Beaty et al.  
5,431,567 A 7/1995 Daftary  
5,437,551 A 8/1995 Chalifoux  
5,440,393 A 8/1995 Wenz  
5,452,219 A 9/1995 Dehoff et al.  
5,458,488 A 10/1995 Chalifoux  
5,476,382 A 12/1995 Daftary  
5,476,383 A 12/1995 Beaty et al.



(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,492,471 A	2/1996	Singer	6,099,311 A	8/2000	Wagner et al.
5,497,336 A	3/1996	Andersson et al.	6,099,313 A	8/2000	Dorken et al.
5,516,288 A	5/1996	Sichler et al.	6,099,314 A	8/2000	Kopelman et al.
5,527,182 A *	6/1996	Willoughby ..... A61C 8/0001	6,120,293 A	9/2000	Lazzara et al.
		433/172	6,129,548 A	10/2000	Lazzara et al.
5,533,898 A	7/1996	Mena	6,135,773 A	10/2000	Lazzara
5,538,426 A	7/1996	Harding et al.	6,142,782 A	11/2000	Lazarof
5,547,377 A	8/1996	Daftary	6,159,010 A	12/2000	Rogers et al.
5,556,278 A	9/1996	Meitner	6,174,168 B1	1/2001	Dehoff et al.
5,564,921 A	10/1996	Marlin	6,175,413 B1	1/2001	Lucas
5,564,924 A	10/1996	Kwan	6,190,169 B1	2/2001	Bluemli et al.
5,569,578 A	10/1996	Mushabac	6,197,410 B1	3/2001	Vallittu et al.
5,575,656 A	11/1996	Hajjar	6,200,125 B1	3/2001	Akutagawa
5,580,244 A	12/1996	White	6,206,693 B1	3/2001	Hultgren
5,580,246 A	12/1996	Fried et al.	6,210,162 B1	4/2001	Chishti et al.
5,595,703 A	1/1997	Swaelens et al.	6,217,331 B1	4/2001	Rogers et al.
5,613,832 A	3/1997	Su	6,217,334 B1	4/2001	Hultgren
5,613,852 A	3/1997	Bavitz	6,227,859 B1	5/2001	Sutter
5,616,899 A	4/1997	Recigno	6,244,867 B1	6/2001	Aravena et al.
5,630,717 A	5/1997	Zuest et al.	6,257,890 B1	7/2001	Khoury et al.
5,636,986 A	6/1997	Pezeshkian	6,273,720 B1	8/2001	Spalten
5,651,675 A	7/1997	Singer	6,283,753 B1	9/2001	Willoughby
5,652,709 A	7/1997	Andersson et al.	6,287,119 B1	9/2001	Van Nifterick et al.
5,658,147 A	8/1997	Phimmasone	6,296,483 B1	10/2001	Champleboux
5,662,476 A	9/1997	Ingber et al.	6,305,939 B1	10/2001	Dawood
5,674,069 A	10/1997	Osorio	6,312,260 B1	11/2001	Kumar
5,674,071 A	10/1997	Beaty et al.	6,319,000 B1	11/2001	Branemark
5,674,073 A	10/1997	Ingber et al.	6,322,728 B1	11/2001	Brodkin et al.
5,681,167 A	10/1997	Lazarof	6,334,853 B1	1/2002	Kopelman
5,685,715 A	11/1997	Beaty et al.	6,358,052 B1	3/2002	Lustig et al.
5,688,283 A	11/1997	Knapp	6,382,975 B1	5/2002	Poirier
5,704,936 A	1/1998	Mazel	6,402,707 B1	6/2002	Ernst
5,718,579 A	2/1998	Kennedy	6,406,295 B1 *	6/2002	Mahler ..... A61C 8/00
5,725,376 A	3/1998	Poirier			433/173
5,733,123 A	3/1998	Blacklock et al.	6,431,866 B2	8/2002	Hurson et al.
5,733,124 A	3/1998	Kwan	6,431,867 B1	8/2002	Gittelsohn et al.
5,741,215 A	4/1998	D'urso	6,488,503 B1	12/2002	Lichkus et al.
5,743,916 A	4/1998	Greenberg et al.	6,497,574 B1	12/2002	Miller
5,759,036 A *	6/1998	Hinds ..... A61C 8/005	6,514,258 B1	2/2003	Brown et al.
		433/172	6,540,784 B2	4/2003	Barlow et al.
5,762,125 A	6/1998	Mastrorrio	6,558,162 B1	5/2003	Porter et al.
5,762,500 A	6/1998	Lazarof	6,568,936 B2	5/2003	Macdougald et al.
5,768,134 A	6/1998	Swaelens et al.	6,575,751 B1	6/2003	Lehmann et al.
5,769,636 A	6/1998	Di Sario	6,594,539 B1	7/2003	Geng
5,791,902 A	8/1998	Lauks	6,610,079 B1	8/2003	Li et al.
5,800,168 A	9/1998	Cascione et al.	6,619,958 B2	9/2003	Beaty et al.
5,810,592 A	9/1998	Daftary	6,629,840 B2	10/2003	Chishti et al.
5,813,858 A	9/1998	Singer	6,634,883 B2	10/2003	Ranalli
5,823,778 A	10/1998	Schmitt et al.	6,644,970 B1	11/2003	Lin et al.
5,842,859 A	12/1998	Palacci	6,648,640 B2	11/2003	Rubbert et al.
5,846,079 A	12/1998	Knode	6,671,539 B2	12/2003	Gateno et al.
5,851,115 A	12/1998	Carlsson et al.	6,672,870 B2	1/2004	Knapp
5,857,853 A	1/1999	Van Nifterick et al.	6,688,887 B2	2/2004	Morgan
5,871,358 A	2/1999	Ingber et al.	6,691,764 B2	2/2004	Embert et al.
5,873,722 A	2/1999	Lazzara et al.	6,726,480 B1	4/2004	Sutter
5,876,204 A	3/1999	Day et al.	6,743,491 B2	6/2004	Cirincione et al.
5,885,078 A	3/1999	Cagna et al.	6,755,652 B2	6/2004	Nanni
5,888,034 A	3/1999	Greenberg	6,772,026 B2	8/2004	Bradbury et al.
5,902,109 A	5/1999	Reams, III et al.	6,776,614 B2	8/2004	Wiechmann et al.
5,904,483 A	5/1999	Wade	6,783,359 B2	8/2004	Kapit
5,915,962 A	6/1999	Rosenlicht	6,790,040 B2	9/2004	Amber et al.
5,927,982 A	7/1999	Kruger	6,793,491 B2	9/2004	Klein et al.
5,938,443 A	8/1999	Lazzara et al.	6,808,659 B2	10/2004	Schulman et al.
5,954,769 A	9/1999	Rosenlicht	6,814,575 B2	11/2004	Poirier
5,964,591 A	10/1999	Beaty et al.	6,821,462 B2	11/2004	Schulman et al.
5,967,777 A	10/1999	Klein et al.	6,829,498 B2	12/2004	Kipke et al.
5,984,681 A	11/1999	Huang	D503,804 S	4/2005	Phleps et al.
5,989,025 A	11/1999	Conley	6,882,894 B2	4/2005	Durbin et al.
5,989,029 A	11/1999	Osorio et al.	6,885,464 B1	4/2005	Pfeiffer et al.
5,989,258 A	11/1999	Hattori	6,902,401 B2	6/2005	Jornéus et al.
5,997,681 A	12/1999	Kinzie	6,913,463 B2	7/2005	Blacklock
6,000,939 A	12/1999	Ray et al.	6,926,442 B2	8/2005	Stöckl
6,008,905 A	12/1999	Breton et al.	6,926,525 B1	8/2005	Rønvig et al.
6,068,479 A	5/2000	Kwan	6,939,489 B2	9/2005	Moszner et al.
6,093,023 A	7/2000	Sala Meseguer	6,942,699 B2	9/2005	Stone et al.
			6,953,383 B2	10/2005	Rothenberger
			6,957,118 B2	10/2005	Kopelman et al.
			6,966,772 B2	11/2005	Malin et al.
			6,970,760 B2	11/2005	Wolf et al.



(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,971,877 B2	12/2005	Harter	7,628,537 B2	12/2009	Schulze-Ganzlin
6,994,549 B2	2/2006	Brodkin et al.	7,632,097 B2	12/2009	De Clerck
7,010,150 B1	3/2006	Pfeiffer et al.	7,653,455 B2	1/2010	Cinader, Jr.
7,010,153 B2	3/2006	Zimmermann	7,654,823 B2	2/2010	Dadi
7,012,988 B2	3/2006	Adler et al.	7,655,586 B1	2/2010	Brodkin et al.
7,018,207 B2	3/2006	Prestipino	7,658,610 B2	2/2010	Knopp
7,021,934 B2	4/2006	Aravena	7,661,956 B2	2/2010	Powell et al.
7,029,275 B2	4/2006	Rubbert et al.	7,665,989 B2	2/2010	Brajnovic et al.
7,044,735 B2	5/2006	Malin	7,679,723 B2	3/2010	Schwotzer
7,056,115 B2	6/2006	Phan et al.	7,687,754 B2	3/2010	Eiff et al.
7,056,472 B1	6/2006	Behringer	7,689,308 B2	3/2010	Holzner et al.
7,059,856 B2	6/2006	Marotta	D614,210 S	4/2010	Basler et al.
7,066,736 B2	6/2006	Kumar et al.	7,698,014 B2	4/2010	Dunne et al.
7,084,868 B2	8/2006	Farag et al.	7,758,346 B1	7/2010	Letcher
7,086,860 B2	8/2006	Schuman et al.	7,774,084 B2	8/2010	Cinader, Jr.
7,097,451 B2	8/2006	Tang	7,780,907 B2	8/2010	Schmidt et al.
7,104,795 B2	9/2006	Dadi	7,785,007 B2	8/2010	Stoeckl
7,110,844 B2	9/2006	Kopelman et al.	7,787,132 B2	8/2010	Körner et al.
7,112,065 B2	9/2006	Kopelman et al.	7,796,811 B2	9/2010	Orth et al.
7,118,375 B2	10/2006	Durbin et al.	7,798,708 B2	9/2010	Erhardt et al.
D532,991 S	12/2006	Gozzi et al.	7,801,632 B2	9/2010	Orth et al.
7,153,132 B2	12/2006	Tedesco	7,815,371 B2	10/2010	Schulze-ganzlin
7,153,135 B1	12/2006	Thomas	7,824,181 B2	11/2010	Sers
7,163,443 B2	1/2007	Basler et al.	D629,908 S	12/2010	Jerger et al.
7,175,434 B2	2/2007	Brajnovic	7,855,354 B2	12/2010	Eiff et al.
7,175,435 B2	2/2007	Andersson et al.	7,865,261 B2	1/2011	Pfeiffer
7,178,731 B2	2/2007	Basler	7,876,877 B2	1/2011	Stockl
7,214,062 B2	5/2007	Morgan	7,901,209 B2	3/2011	Saliger et al.
7,220,124 B2	5/2007	Taub et al.	7,922,488 B2 *	4/2011	Falk ..... A61C 13/0001 433/173
7,228,191 B2	6/2007	Hofmeister et al.	7,982,731 B2	7/2011	Orth et al.
7,236,842 B2	6/2007	Kopelman et al.	7,985,119 B2	7/2011	Basler et al.
7,281,927 B2	10/2007	Marotta	7,986,415 B2	7/2011	Thiel et al.
7,286,954 B2	10/2007	Kopelman et al.	7,988,449 B2	8/2011	Amber et al.
7,303,420 B2	12/2007	Huch et al.	8,002,547 B2	8/2011	Porter et al.
7,319,529 B2	1/2008	Babayoff	8,011,925 B2	9/2011	Powell et al.
7,322,746 B2	1/2008	Beckhaus et al.	8,011,927 B2	9/2011	Berckmans, III
7,322,824 B2	1/2008	Schmitt	8,026,943 B2	9/2011	Weber et al.
7,324,680 B2	1/2008	Zimmermann	8,033,826 B2	10/2011	Towse et al.
7,329,122 B1	2/2008	Scott	8,038,440 B2	10/2011	Swaelens et al.
7,333,874 B2	2/2008	Taub et al.	8,047,895 B2	11/2011	Basler
7,335,876 B2	2/2008	Eiff et al.	8,057,912 B2	11/2011	Basler et al.
D565,184 S	3/2008	Royzen	8,062,034 B2	11/2011	Hanisch et al.
7,367,801 B2	5/2008	Saliger	8,075,313 B2	12/2011	Ranck et al.
7,379,584 B2	5/2008	Rubbert et al.	8,083,522 B2	12/2011	Karkar et al.
D571,471 S	6/2008	Stöckl	8,105,081 B2	1/2012	Bavar
7,381,191 B2	6/2008	Fallah	8,185,224 B2	5/2012	Powell et al.
7,383,094 B2	6/2008	Kopelman et al.	8,226,654 B2	7/2012	Ranck et al.
D575,747 S	8/2008	Abramovich et al.	8,257,083 B2	9/2012	Berckmans, III et al.
7,421,608 B2	9/2008	Schron	8,353,703 B2	1/2013	Amber et al.
7,425,131 B2	9/2008	Amber et al.	8,944,816 B2 *	2/2015	Robb ..... A61C 8/0048 433/172
7,429,175 B2	9/2008	Gittelsohn	8,944,818 B2	2/2015	Robb et al.
7,435,088 B2	10/2008	Brajnovic	9,629,696 B2	4/2017	Ouellette
7,476,100 B2	1/2009	Kuo	2001/0008751 A1	7/2001	Chishti et al.
7,481,647 B2	1/2009	Sambu et al.	2001/0003401 A1	10/2001	Macdougald et al.
7,488,174 B2	2/2009	Kopelman et al.	2002/0010568 A1	1/2002	Rubbert et al.
7,497,619 B2	3/2009	Stoeckl	2002/0028418 A1	3/2002	Farag et al.
7,497,983 B2	3/2009	Khan et al.	2002/0039717 A1	4/2002	Amber et al.
7,520,747 B2	4/2009	Stonisch	2002/0160337 A1	10/2002	Klein et al.
7,522,764 B2	4/2009	Schwotzer	2002/0001671 A1	11/2002	Moszner et al.
7,534,266 B2	5/2009	Kluger	2003/0082498 A1	5/2003	Halldin et al.
7,536,234 B2	5/2009	Kopelman et al.	2003/0130605 A1	7/2003	Besek
7,545,372 B2	6/2009	Kopelman et al.	2003/0198920 A1	10/2003	Lin
7,551,760 B2	6/2009	Scharlack et al.	2003/0222366 A1	12/2003	Stangel et al.
7,555,403 B2	6/2009	Kopelman et al.	2004/0029074 A1	2/2004	Brajnovic
7,556,496 B2	7/2009	Cinader, Jr. et al.	2004/0048227 A1	3/2004	Brajnovic
7,559,692 B2	7/2009	Beckhaus et al.	2004/0180308 A1	9/2004	Ebi et al.
7,563,397 B2	7/2009	Schulman et al.	2004/0219477 A1	11/2004	Harter
D597,769 S	8/2009	Richter	2004/0219479 A1	11/2004	Malin
7,572,058 B2	8/2009	Pruss et al.	2004/0219490 A1	11/2004	Gartner et al.
7,572,125 B2	8/2009	Brajnovic	2004/0220691 A1	11/2004	Hofmeister et al.
7,574,025 B2	8/2009	Feldman	2004/0241611 A1	12/2004	Amber et al.
7,578,673 B2	8/2009	Wen et al.	2004/0243481 A1	12/2004	Bradbury et al.
7,580,502 B2	8/2009	Dalpiaz et al.	2004/0259051 A1	12/2004	Brajnovic
7,581,951 B2	9/2009	Lehmann et al.	2005/0002371 A1	2/2005	Brodkin et al.
7,582,855 B2	9/2009	Pfeiffer	2005/0056350 A1	3/2005	Dolabdjian et al.
			2005/0070782 A1	3/2005	Brodkin
			2005/0084144 A1	4/2005	Feldman



(56)

## References Cited

## U.S. PATENT DOCUMENTS

2005/0100861 A1 5/2005 Choi et al.  
 2005/0170311 A1 8/2005 Tardieu et al.  
 2005/0271996 A1 12/2005 Sporbert et al.  
 2005/0277089 A1 12/2005 Brajnovic  
 2005/0277090 A1 12/2005 Anderson et al.  
 2005/0277091 A1 12/2005 Andersson et al.  
 2005/0282106 A1 12/2005 Sussman et al.  
 2005/0283065 A1 12/2005 Babayoff  
 2006/0006561 A1 1/2006 Brajnovic  
 2006/0008763 A1 1/2006 Brajnovic  
 2006/0008770 A1 1/2006 Brajnovic et al.  
 2006/0093988 A1 5/2006 Swaelens et al.  
 2006/0094951 A1 5/2006 Dean et al.  
 2006/0127848 A1 6/2006 Sogo et al.  
 2006/0204928 A1 9/2006 Hurson  
 2006/0210949 A1 9/2006 Stoop  
 2006/0263741 A1 11/2006 Imgrund et al.  
 2006/0263747 A1 11/2006 Hurson  
 2006/0281041 A1 12/2006 Rubbert et al.  
 2007/0015111 A1 1/2007 Kopelman et al.  
 2007/0031790 A1 2/2007 Raby et al.  
 2007/0065777 A1 3/2007 Becker  
 2007/0077532 A1 4/2007 Harter  
 2007/0092854 A1 4/2007 Powell et al.  
 2007/0141525 A1 6/2007 Cinader, Jr.  
 2007/0211081 A1 9/2007 Quadling et al.  
 2007/0218426 A1 9/2007 Quadling et al.  
 2007/0269769 A1 11/2007 Marchesi  
 2007/0281277 A1 12/2007 Brajnovic  
 2007/0298377 A1 12/2007 Kenealy et al.  
 2008/0038692 A1 2/2008 Andersson et al.  
 2008/0044794 A1 2/2008 Brajnovic  
 2008/0057467 A1 3/2008 Gittelsohn  
 2008/0070181 A1 3/2008 Abolfathi et al.  
 2008/0009021 A1 4/2008 Brajnovic  
 2008/0085489 A1 4/2008 Schmitt  
 2008/0114371 A1 5/2008 Kluger  
 2008/0118895 A1 5/2008 Brajnovic  
 2008/0124676 A1 5/2008 Marotta  
 2008/0153060 A1 6/2008 De Moyer  
 2008/0153061 A1 6/2008 Marcello  
 2008/0153065 A1 6/2008 Brajnovic et al.  
 2008/0153067 A1 6/2008 Berckmans et al.  
 2008/0153069 A1 6/2008 Holzner et al.  
 2008/0176189 A1 7/2008 Stonisch  
 2008/0206714 A1 8/2008 Schmitt  
 2008/0233537 A1 \* 9/2008 Amber ..... A61C 9/004  
 433/173  
 2008/0233539 A1 9/2008 Rossler  
 2008/0241798 A1 10/2008 Holzner et al.  
 2008/0261165 A1 10/2008 Steingart et al.  
 2008/0261176 A1 10/2008 Hurson  
 2008/0286722 A1 11/2008 Berckmans, III et al.  
 2008/0300716 A1 12/2008 Kopelman et al.  
 2009/0017418 A1 1/2009 Gittelsohn  
 2009/0026643 A1 1/2009 Wiest et al.  
 2009/0042167 A1 2/2009 Van Der Zel  
 2009/0081616 A1 3/2009 Pfeiffer  
 2009/0009851 A1 4/2009 Zhang  
 2009/0087817 A1 4/2009 Jansen et al.  
 2009/0092948 A1 4/2009 Gantes  
 2009/0098511 A1 4/2009 Zhang  
 2009/0060415 A1 5/2009 Galgut et al.  
 2009/0123045 A1 5/2009 Quadling et al.  
 2009/0123887 A1 5/2009 Brajnovic  
 2009/0130629 A1 5/2009 Towse et al.  
 2009/0130630 A1 5/2009 Suttin et al.  
 2009/0186319 A1 7/2009 Sager  
 2009/0187393 A1 7/2009 Van Lierde et al.  
 2009/0220134 A1 9/2009 Cahill et al.  
 2009/0220916 A1 9/2009 Fisker et al.  
 2009/0220917 A1 9/2009 Jensen  
 2009/0239197 A1 9/2009 Brajnovic  
 2009/0239200 A1 9/2009 Brajnovic et al.  
 2009/0253097 A1 10/2009 Brajnovic

2009/0263764 A1 10/2009 Berckmans, III et al.  
 2009/0287332 A1 11/2009 Adusumilli et al.  
 2009/0298009 A1 12/2009 Brajnovic  
 2009/0298017 A1 12/2009 Boerjes et al.  
 2009/0317763 A1 12/2009 Brajnovic  
 2009/0325122 A1 12/2009 Brajnovic et al.  
 2010/0009314 A1 1/2010 Tardieu et al.  
 2010/0028827 A1 2/2010 Andersson et al.  
 2010/0038807 A1 2/2010 Brodtkin et al.  
 2010/0075275 A1 3/2010 Brajnovic  
 2010/0092904 A1 4/2010 Esposti et al.  
 2010/0105008 A1 4/2010 Powell et al.  
 2010/0151420 A1 6/2010 Ranck  
 2010/0151423 A1 6/2010 Ranck et al.  
 2010/0173260 A1 7/2010 Sogo et al.  
 2010/0209877 A1 8/2010 Hogan et al.  
 2010/0216092 A1 8/2010 Garcia et al.  
 2010/0266985 A1 10/2010 Yau et al.  
 2010/0280798 A1 11/2010 Pattijn et al.  
 2010/0285427 A1 11/2010 Hung  
 2011/0008751 A1 1/2011 Pettersson  
 2011/0060558 A1 3/2011 Pettersson et al.  
 2011/0086327 A1 4/2011 Lerner et al.  
 2011/0129792 A1 6/2011 Berckmans, III et al.  
 2011/0183289 A1 \* 7/2011 Powell ..... G06F 30/00  
 433/173  
 2011/0183290 A1 7/2011 Galgut et al.  
 2011/0191081 A1 8/2011 Malfliet et al.  
 2011/0244426 A1 10/2011 Amber et al.  
 2011/0269104 A1 11/2011 Berckmans, III et al.  
 2011/0275032 A1 11/2011 Tardieu et al.  
 2011/0306008 A1 12/2011 Suttin  
 2011/0306009 A1 12/2011 Suttin et al.  
 2011/0306014 A1 \* 12/2011 Conte ..... A61C 8/005  
 433/173  
 2012/0010740 A1 1/2012 Swaelens et al.  
 2012/0077149 A1 3/2012 Ospelt et al.  
 2012/0135370 A1 5/2012 Ranck et al.  
 2012/0164593 A1 6/2012 Bavar  
 2012/0164893 A1 6/2012 Mitsuzuka et al.  
 2012/0214130 A1 8/2012 Krivoruk  
 2012/0214132 A1 8/2012 Takahashi et al.  
 2012/0264081 A1 10/2012 Philibin  
 2012/0295223 A1 \* 11/2012 Robb ..... A61C 8/006  
 433/173  
 2012/0295226 A1 11/2012 Robb et al.  
 2012/0330315 A1 12/2012 Ranck et al.  
 2013/0171584 A1 7/2013 Brun  
 2013/0189646 A1 7/2013 Hochman et al.  
 2013/0196290 A1 \* 8/2013 Herrington ..... A61C 8/0001  
 433/173  
 2013/0296813 A2 11/2013 Park  
 2013/0309630 A1 11/2013 Bolleter  
 2014/0234801 A1 8/2014 Herrington et al.  
 2014/0343706 A1 11/2014 Hart et al.  
 2015/0104756 A1 4/2015 Robb et al.

## FOREIGN PATENT DOCUMENTS

DE 4028855 A1 3/1992  
 DE 10029256 A1 11/2000  
 EP 0442855 A1 8/1991  
 EP 0583829 A1 2/1994  
 EP 0657146 A1 6/1995  
 EP 0727193 A1 8/1996  
 EP 0747017 A2 12/1996  
 EP 2130514 A1 12/2009  
 EP 2351536 A1 \* 8/2011 ..... A61C 8/0001  
 FR 2759896 A3 8/1998  
 GB 1291470 A 10/1972  
 JP 05212063 A 8/1993  
 JP 06154252 A 6/1994  
 JP 09218916 A 8/1997  
 JP 2000512882 A 10/2000  
 JP 2003190187 A 7/2003  
 JP 2003524481 A 8/2003  
 JP 2006512172 A 4/2006  
 JP 2009512533 A 3/2009



(56)

**References Cited**

## FOREIGN PATENT DOCUMENTS

KR	20100090564	A	8/2010
KR	10110828081		1/2012
WO	WO-8502337	A1	6/1985
WO	WO-9426200A	1	11/1994
WO	WO-1994026200	A1	11/1994
WO	WO-1999032045	A1	7/1999
WO	WO-2000008415	A1	2/2000
WO	WO-0134057	A1	5/2001
WO	WO-2001058379	A1	8/2001
WO	WO-2002053055	A1	7/2002
WO	WO-2003024352	A1	3/2003
WO	WO-2004030565	A1	4/2004
WO	WO-2004075771	A1	9/2004
WO	WO-2004087000	A1	10/2004
WO	WO-2004098435	A2	11/2004
WO	WO-2006014130	A1	2/2006
WO	WO-2006062459	A1	6/2006
WO	WO-2006082198	A1	8/2006
WO	WO-2007005490	A2	1/2007
WO	WO-2007033157	A2	3/2007
WO	WO-2007104842	A1	9/2007
WO	WO-2007129955	A1	11/2007
WO	WO-2008057955	A2	5/2008
WO	WO-2008083857	A1	7/2008
WO	WO-2009060415	A2	5/2009
WO	WO-2009146164	A1	12/2009
WO	WO-2010088754	A1	8/2010
WO	WO-2012126475	A1	9/2012

## OTHER PUBLICATIONS

“U.S. Appl. No. 13/798,894, Advisory Action dated Nov. 9, 2018”, 3 pgs.  
 “U.S. Appl. No. 13/798,894, Appeal Brief filed Jul. 13, 2015”, 23 pgs.  
 “U.S. Appl. No. 13/798,894, Appeal Decision dated Jul. 24, 2017”, 16 pgs.  
 “U.S. Appl. No. 13/798,894, Examiner’s Answer dated Oct. 6, 2015”, 11 pgs.  
 “U.S. Appl. No. 13/798,894, Final Office Action dated Jan. 13, 2015”, 12 pgs.  
 “U.S. Appl. No. 13/798,894, Final Office Action dated Aug. 28, 2018”, 12 pgs.  
 “U.S. Appl. No. 13/798,894, Non Final Office Action dated Jan. 10, 2019”, 10 pgs.  
 “U.S. Appl. No. 13/798,894, Non Final Office Action dated Jan. 12, 2018”, 14 pgs.  
 “U.S. Appl. No. 13/798,894, Non Final Office Action dated Aug. 26, 2014”, 15 pgs.  
 “U.S. Appl. No. 13/798,894, Notice of Non-Compliant Amendment dated Oct. 2, 2017”, 2 pgs.  
 “U.S. Appl. No. 13/798,894, Reply Brief filed Nov. 3, 2015”, 6 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Apr. 12, 2018 to Non Final Office Action dated Jan. 12, 2018”, 14 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Apr. 13, 2015 to Final Office Action dated Jan. 13, 2015”, 19 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Jun. 25, 2014 to Restriction Requirement dated Jun. 4, 2014”, 9 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Sep. 26, 2017 to Appeal Decision dated Jul. 24, 2017”, 11 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Oct. 29, 2018 to Final Office Action dated Aug. 28, 2018”, 13 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Nov. 28, 2018 to Advisory Action dated Nov. 11, 2018”, 14 pgs.  
 “European Application Serial No. 19196489.9, Extended European Search Report dated Oct. 30, 2020”, 10 pgs.  
 “European Application Serial No. 19197877.4, Extended European Search Report dated Jan. 12, 2021”, 8 pages.  
 “European Application Serial No. 19196489.9, Response filed Nov. 23, 2021”, 33 pgs.

“European Application Serial No. 19197877.4, Response to Extended European Search Report dated Jan. 12, 2021”, 18 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Dec. 4, 2014 to Non Final Office Action dated Aug. 26, 2014”, 4 pgs.  
 “U.S. Appl. No. 13/798,894, Response filed Feb. 4, 2017 to Notice of Non-Compliant Amendment dated Oct. 2, 2017” 8 pgs.  
 “U.S. Appl. No. 13/798,894, Restriction Requirement dated Jun. 4, 2014”, 7 pgs.  
 “U.S. Appl. No. 14/575,717, Final Office Action dated Apr. 6, 2018”, 18 pgs.  
 “U.S. Appl. No. 14/575,717, Non Final Office Action dated Feb. 23, 2017”, 18 pgs.  
 “U.S. Appl. No. 14/575,717, Non Final Office Action dated Aug. 14, 2018”, 19 pgs.  
 “U.S. Appl. No. 14/575,717, Notice of Allowance dated Mar. 14, 2019”, 12 pgs.  
 “U.S. Appl. No. 14/575,717, Preliminary Amendment filed Dec. 18, 2014”, 8 pgs.  
 “U.S. Appl. No. 14/575,717, Response filed May 23, 2017 to Non Final Office Action dated Feb. 23, 2017”, 6 pgs.  
 “U.S. Appl. No. 14/575,717, Response filed Jul. 6, 2018 to Final Office Action, dated Apr. 6, 2018”, 18 pgs.  
 “U.S. Appl. No. 14/575,717, Response filed Nov. 14, 2018 to Non Final Office Action dated Aug. 14, 2018”, 6 pgs.  
 “U.S. Appl. No. 14/575,717, Response filed Dec. 7, 2016 to Restriction Requirement dated Oct. 7, 2016”, pgs.  
 “U.S. Appl. No. 14/575,717, Restriction Requirement dated Oct. 7, 2016”, 6 pgs.  
 “U.S. Appl. No. 14/575,717, Second Preliminary Amendment filed Dec. 19, 2014”, 6 pgs.  
 “U.S. Appl. No. 14/575,717, Third Preliminary Amendment filed Mar. 17, 2015”, 6 pgs.  
 “Australian Application Serial No. 2015201244, First Examiner Report dated Mar. 14, 2016”, 3 pgs.  
 “Australian Application Serial No. 2015201244, Response filed Jan. 5, 2017 to First Examiner Report dated Mar. 14, 2016”, 63 pgs.  
 “Canadian Application Serial No. 2,833,215, Office Action dated Mar. 10, 2017”, 3 pgs.  
 “Canadian Application Serial No. 2,833,215, Office Action, dated May 3, 2016”, 3 pgs.  
 “Canadian Application Serial No. 2,833,215, Response filed Mar. 28, 2017 to Office Action dated Mar. 10, 2017”, 6 gs.  
 “Canadian Application Serial No. 2,833,215, Response filed Nov. 3, 2016 to Office Action dated May 3, 2016”, 33 pgs.  
 “European Application Serial No. 12786777.8, Communication Pursuant to Article 94(3) EPC dated Dec. 4, 2017”, 7 pgs.  
 “European Application Serial No. 12786777.8, Extended European Search Report dated Oct. 28, 2014”, 7 pgs.  
 “European Application Serial No. 12786777.8, Response filed May 26, 2015 to Extended European Search reportmailed May 26, 2015”, 11 pgs.  
 “European Application Serial No. 12786777.8, Response filed Jun. 25, 2018 to Communication Pursuant to Article 94(3) EPC dated Dec. 14, 2017”, 14 pgs.  
 “European Application Serial No. 1476455.9, Communication Pursuant to Article 94(3) EPC dated Jul. 2, 2018”, 9 pgs.  
 “European Application Serial No. 14776455.9, Extended European Search Report dated Oct. 17, 2016”, 9 pgs.  
 “European Application Serial No. 1476455.9, Response Filed Dec. 19, 2018 to Communication Pursuant to Article 94(3) EPC dated Jul. 2, 2018”, 16 pgs.  
 “International Application Serial No. PCT/US2009/034463, International Search Report dated Apr. 30, 2009”, 2 pgs.  
 “International Application Serial No. PCT/US2009/034463, Written Opinion dated Apr. 20, 2009”. 6 pgs.  
 “International Application Serial No. PCT/US2012/038097, International Search Report dated Sep. 7, 2012”, 2 pgs.  
 “International Application Serial No. PCT/US2012/038097, Written Opinion dated Sep. 7, 2012”, 9 pgs.  
 “International Application Serial No. PCT/US2014/017929, International Search Report dated May 16, 2014”, 2 pgs.  
 “International Application Serial No. PCT/US2014/017929, Written Opinion dated May 16, 2014”, 6 pgs.

(56)

**References Cited**

OTHER PUBLICATIONS

“Japanese Application Serial No. 2014-511483, Office Action dated Jul. 14, 2015”, W/ English Translation, 5 pgs.

“Navigator™ System For CT Guided Surgery Manual”, BIOMET31, (2007), 34 pgs.

“Robots are ready for medical manufacturing”. Retrieved from MachineDesign.com, URL: <http://machinedesign.com/article/robots-are-ready-for-medicalmanufacturing-07122>. (Jul. 12, 2007), 7 pgs.



“Surgical Glue May Help to Eliminate Suturing for Implants”, MedNEWS, Retrieved from MediNEWS. Direct, (Dec. 21, 2007) 1 pg.

Brief, Jakob, et al., “Accuracy of image-guided implantology”, Retrieved from Google: <URL [sitemaker.umnich.edu/sarmentlab/files/robodentsdenxcor05.odf](http://sitemaker.umnich.edu/sarmentlab/files/robodentsdenxcor05.odf)>, (Aug. 20, 2004), 7 pgs.

Goulette, Francois, “A New Method and a Clinical case for Computer Assisted Dental Implantology”. Retrieved from Summer European university in surgical Robotics., [Online] retrieved from the internet: <URL: [www.linnm.frimanifs/UEE/docs/students/goulette.pdf](http://www.linnm.frimanifs/UEE/docs/students/goulette.pdf)>, (Sep. 6, 2003), 7 pgs.

\* cited by examiner



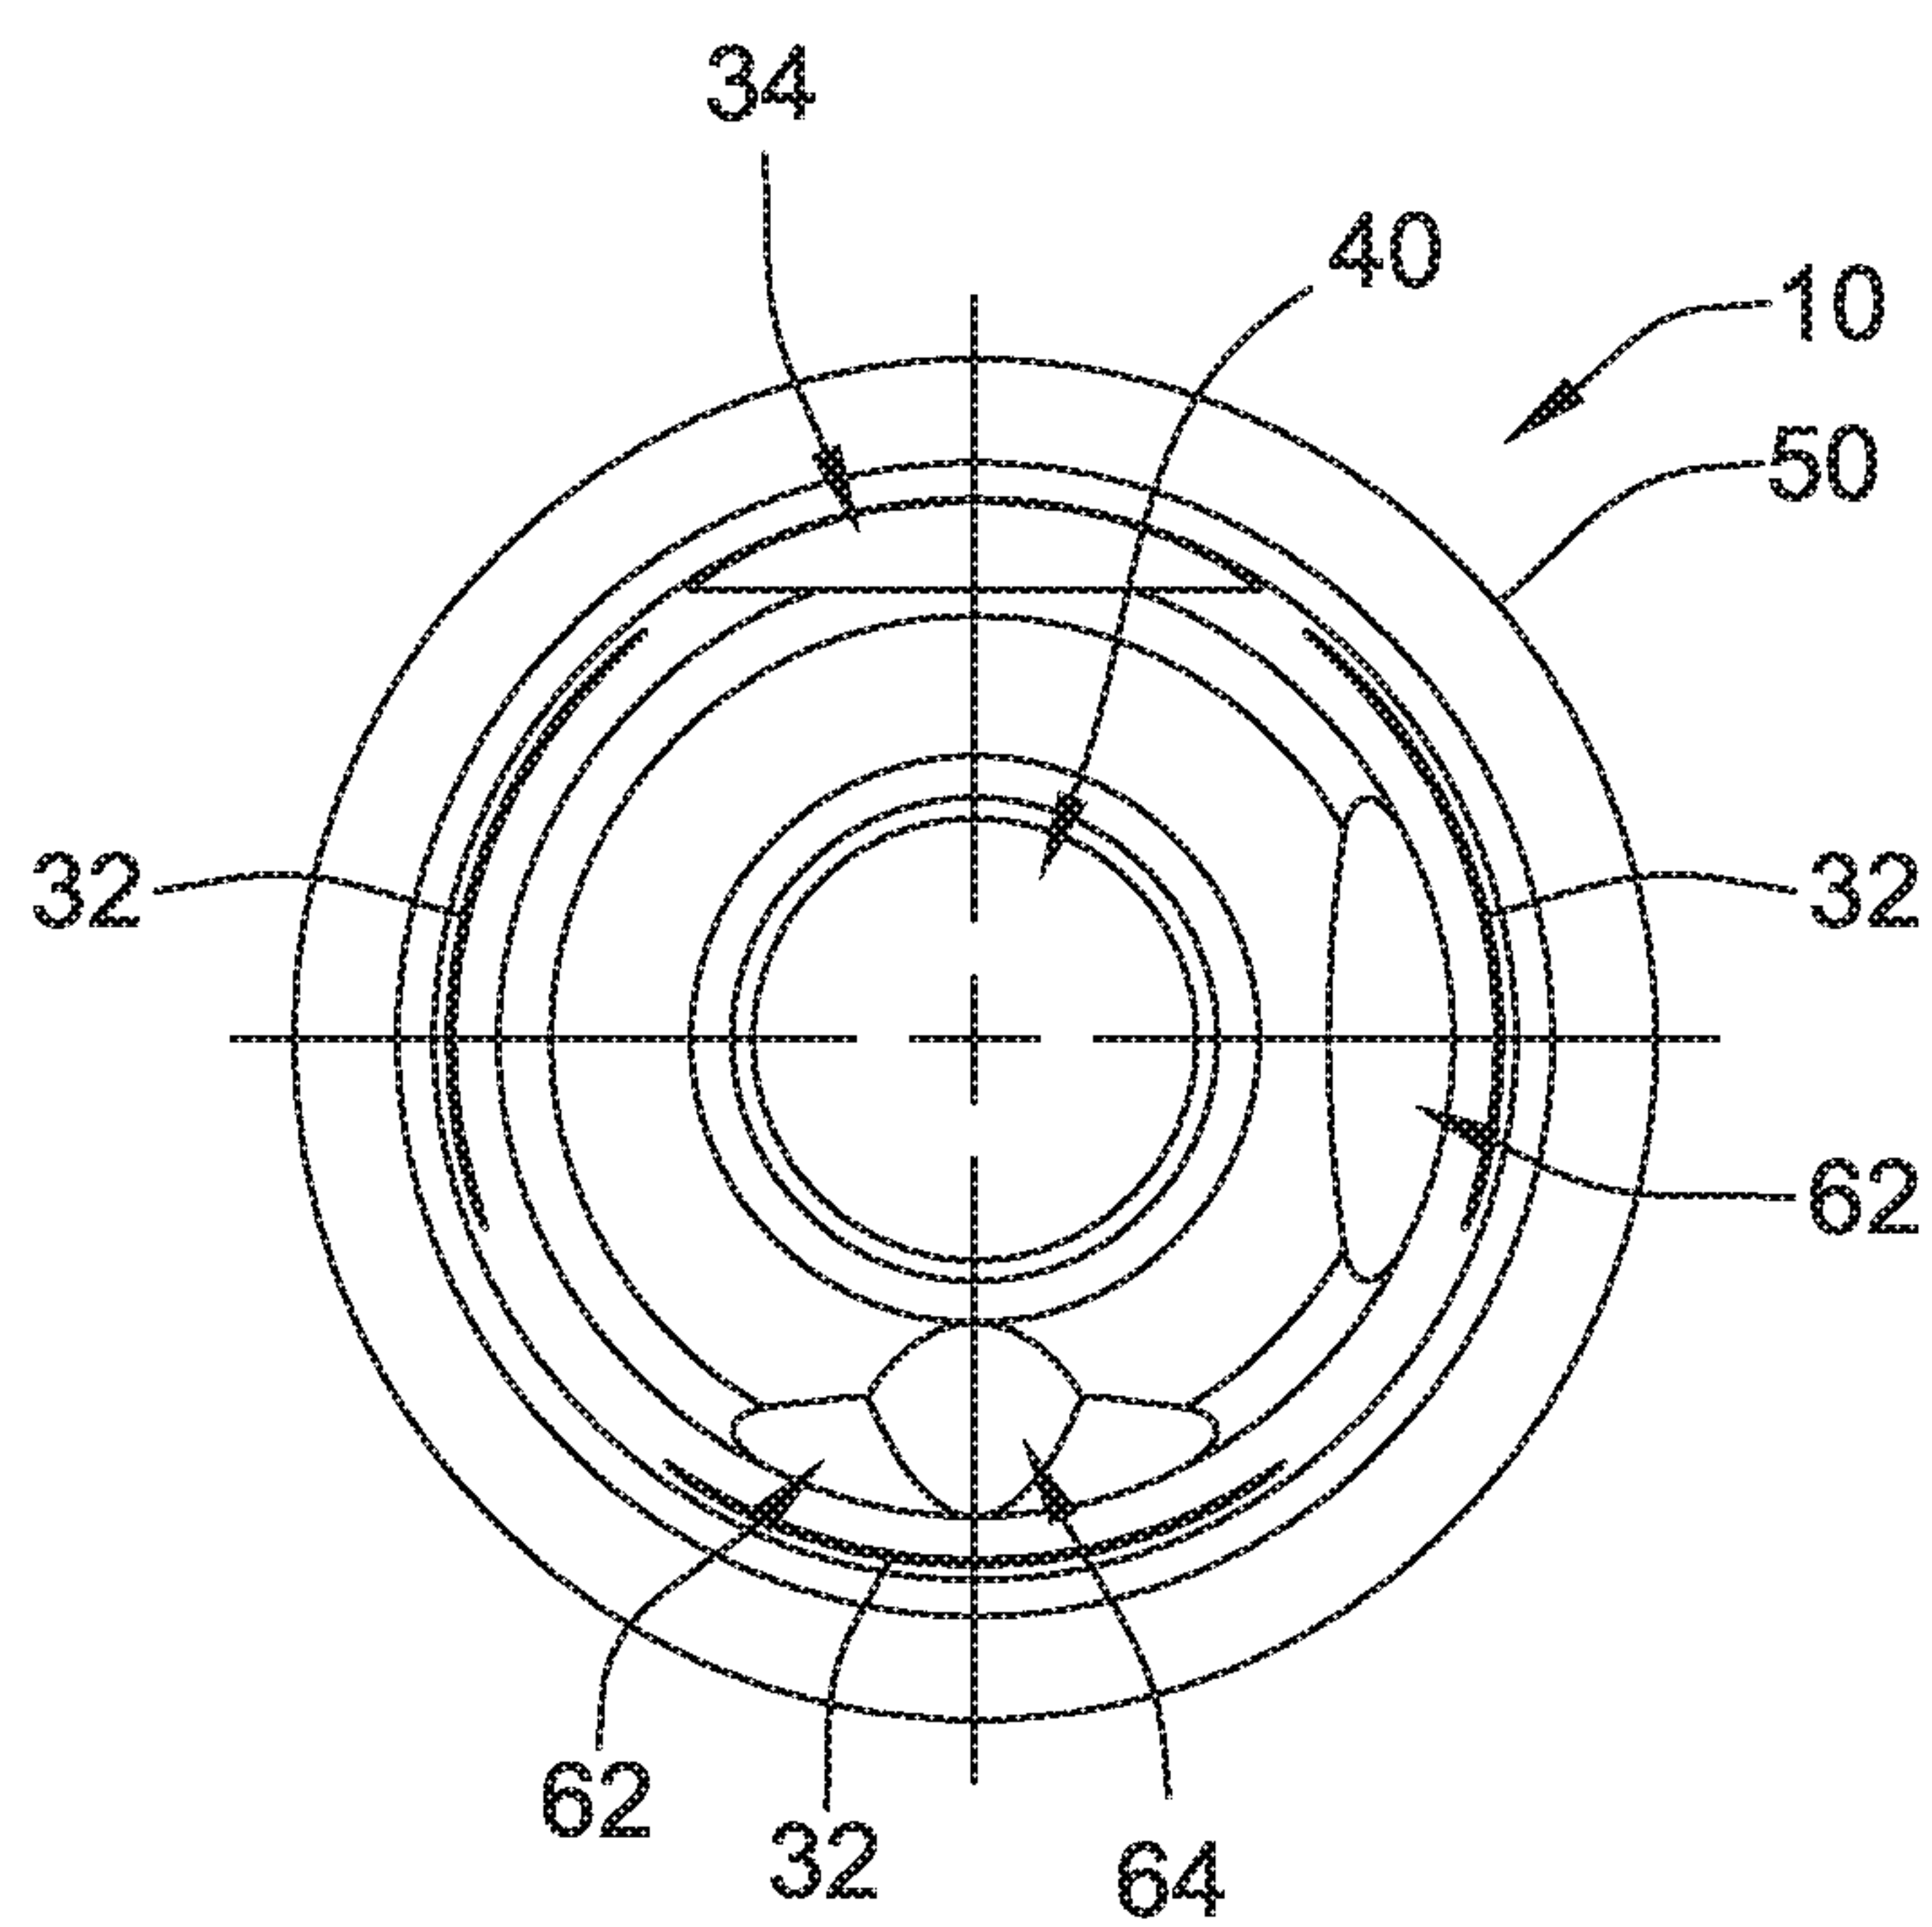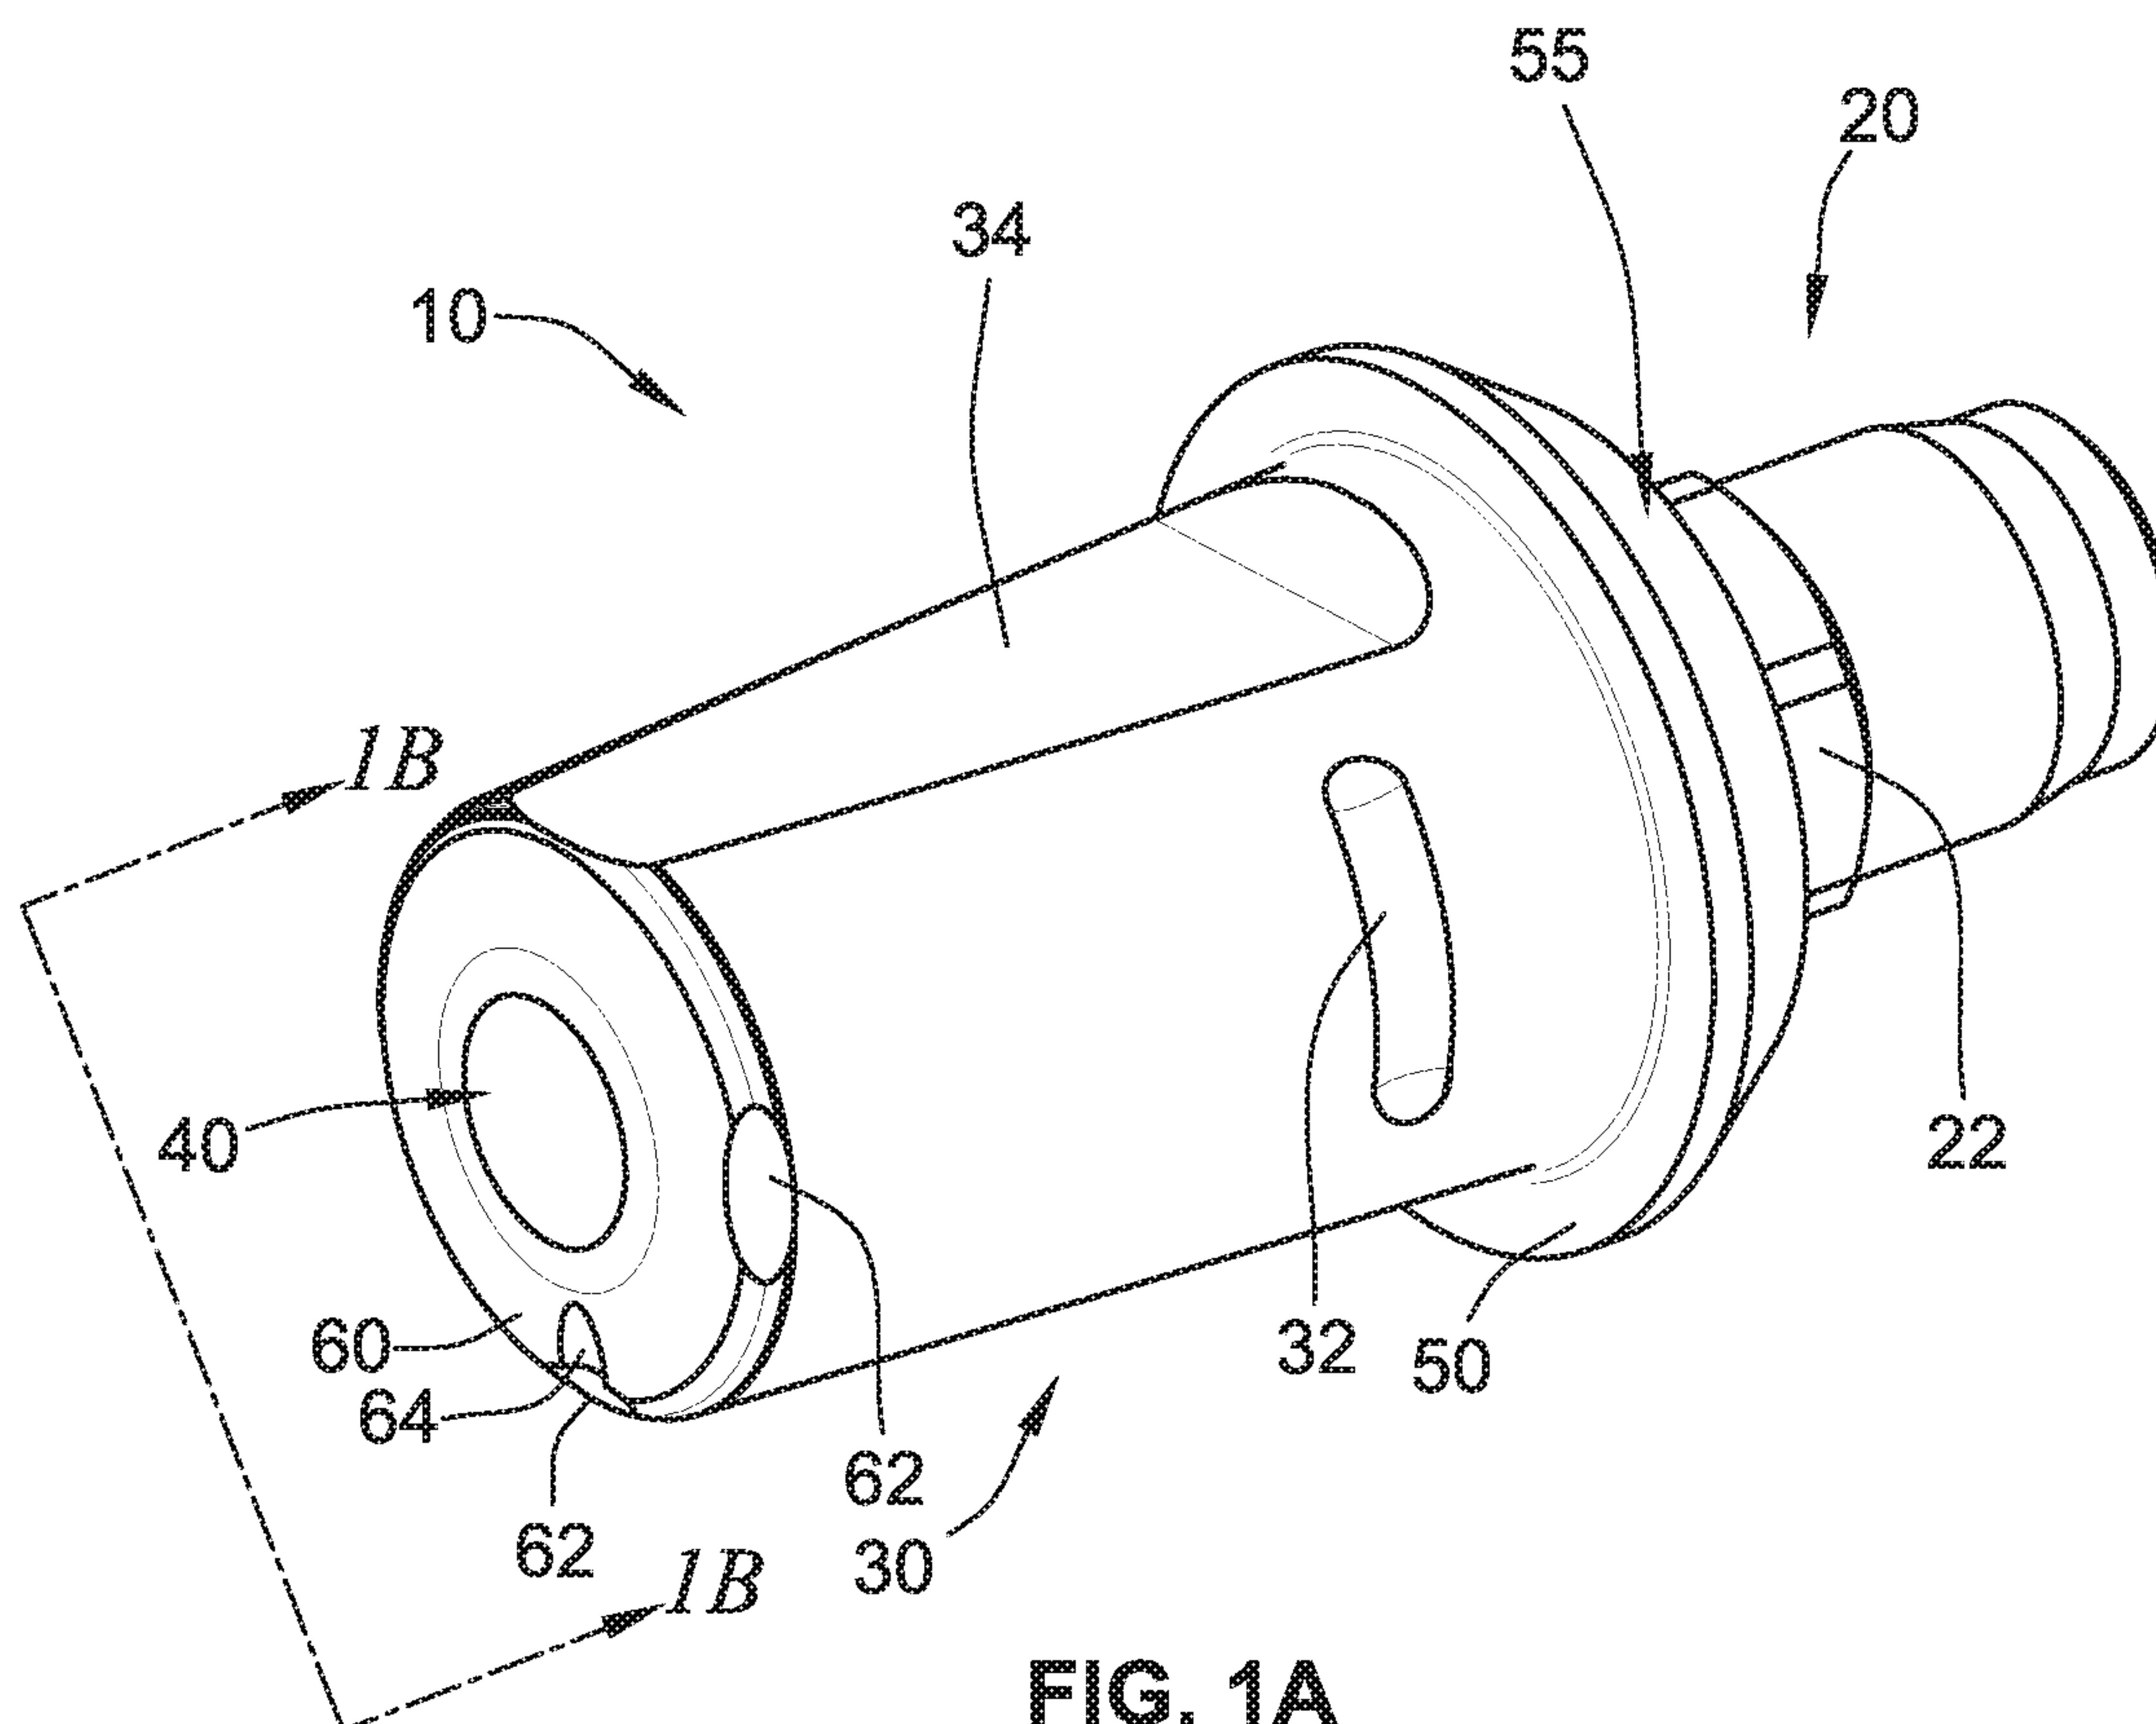



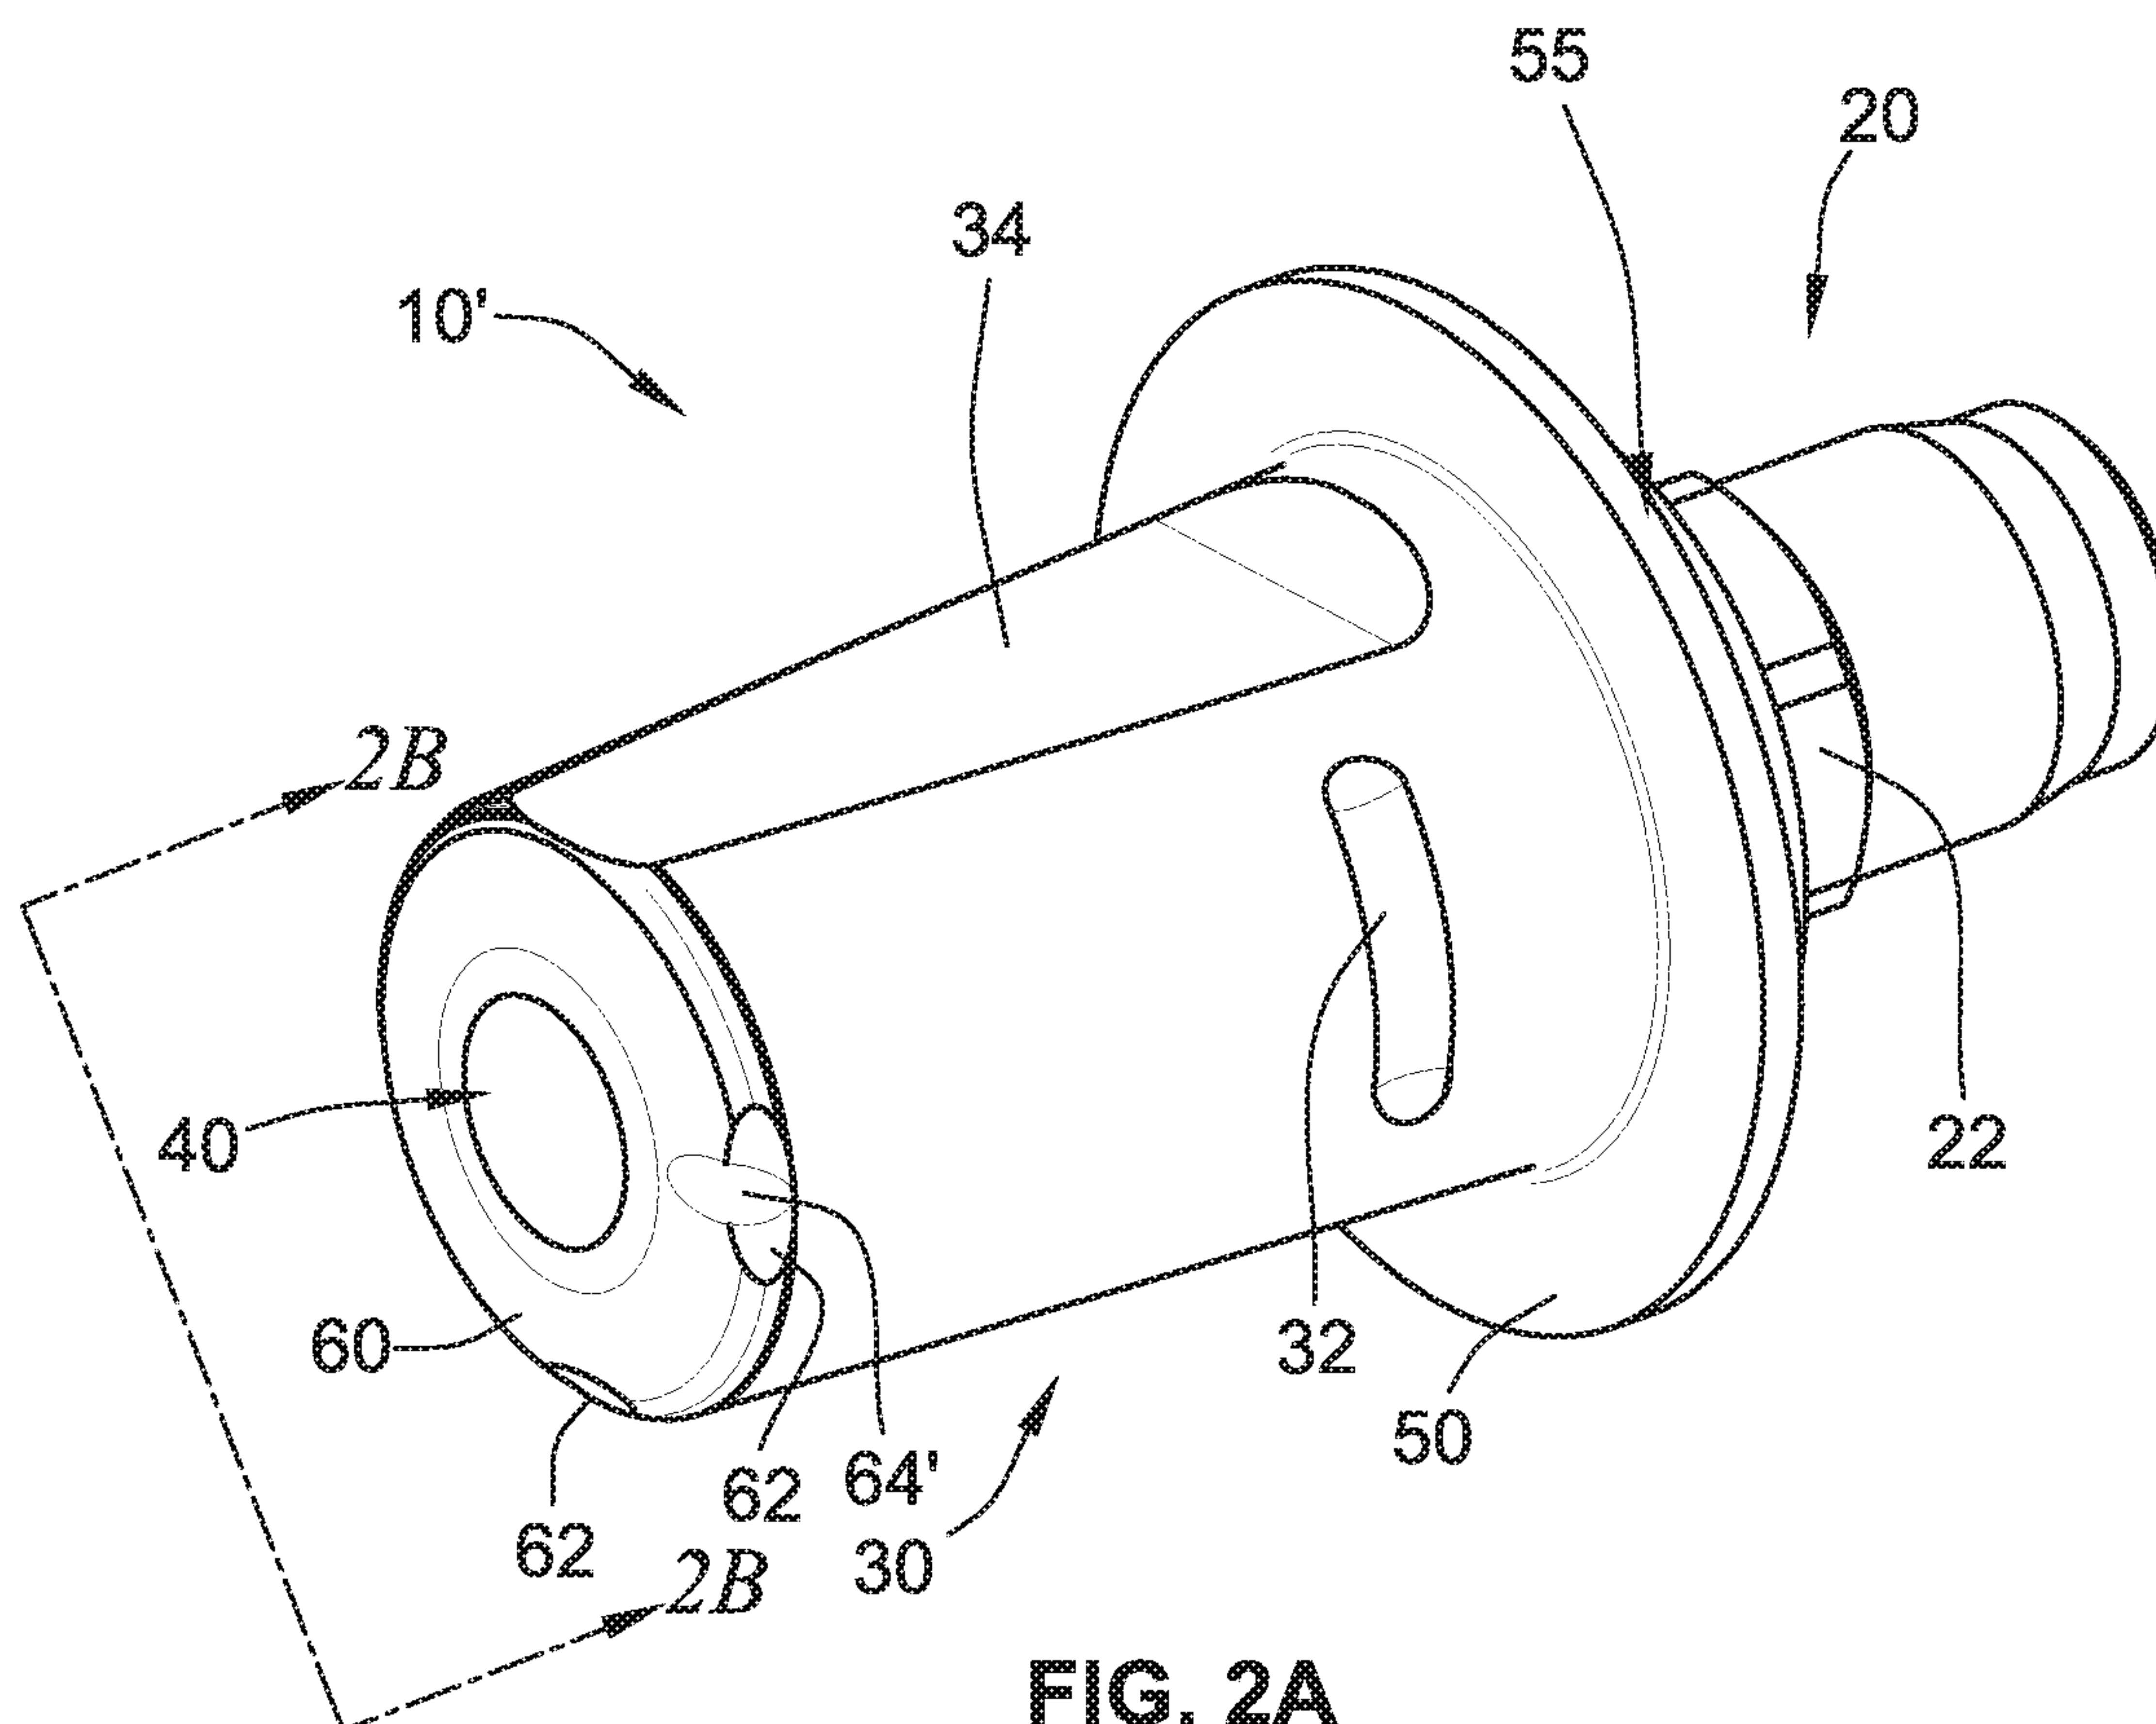


FIG. 2A

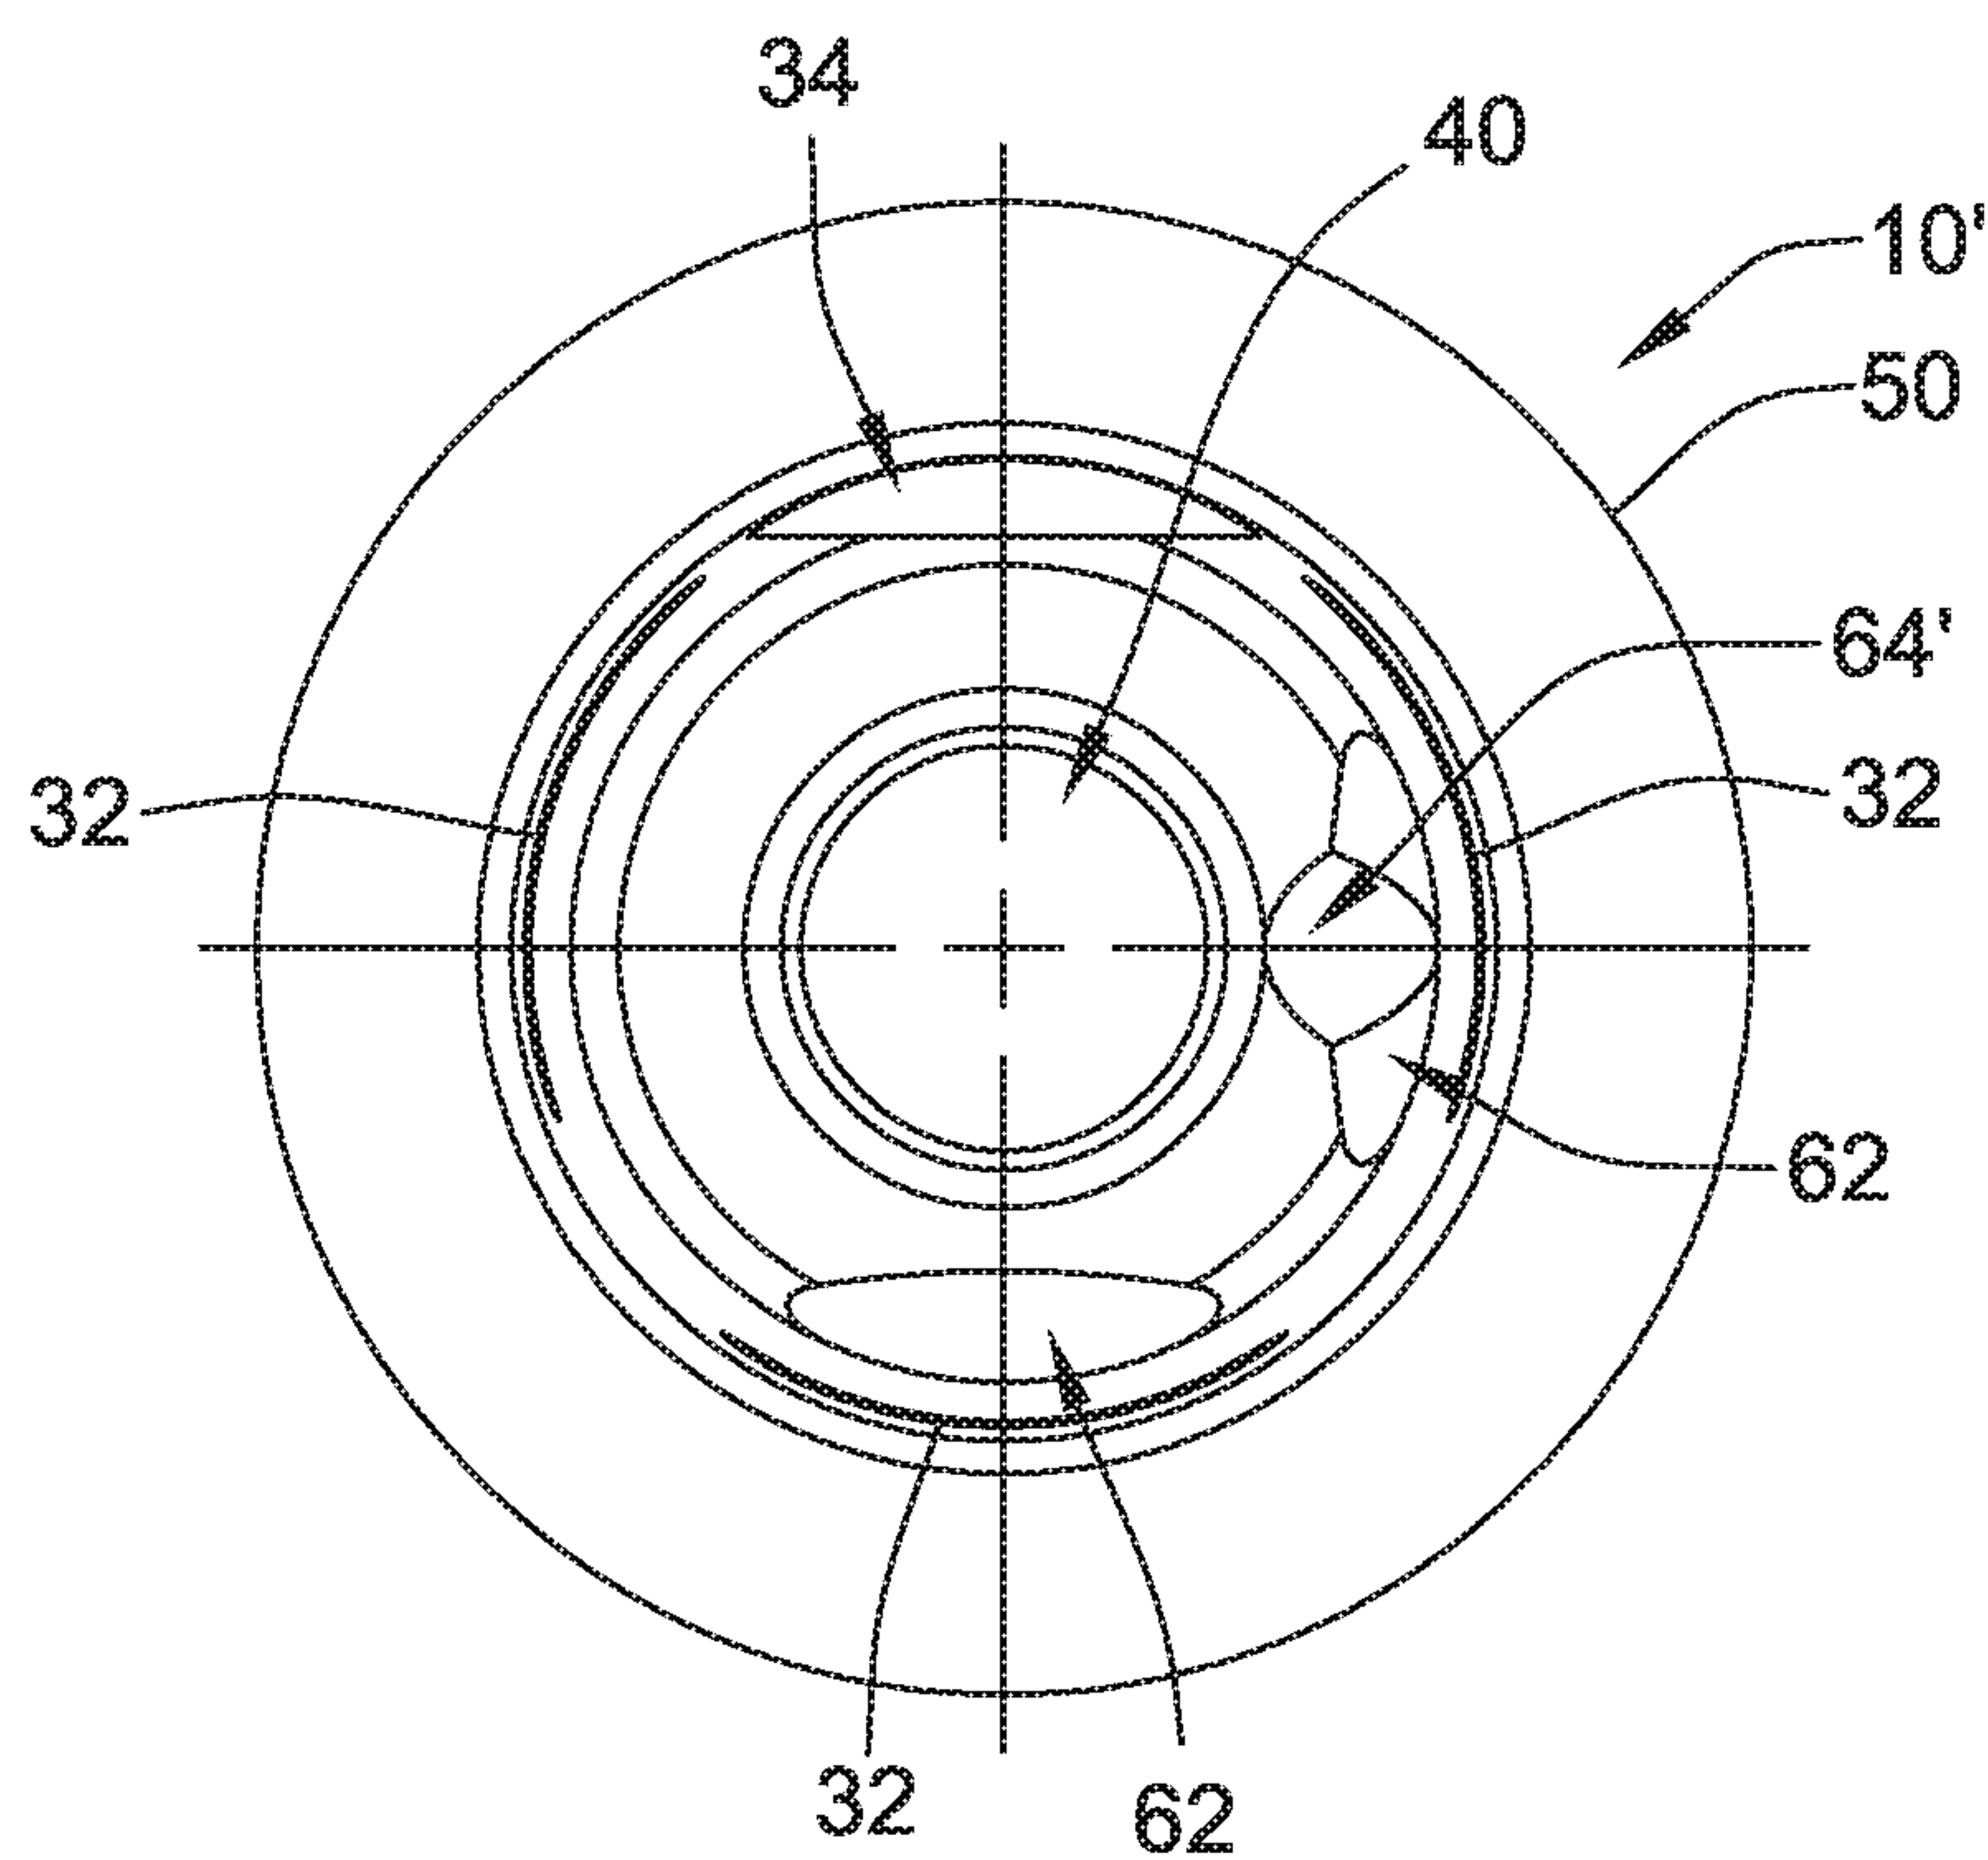


FIG. 2B

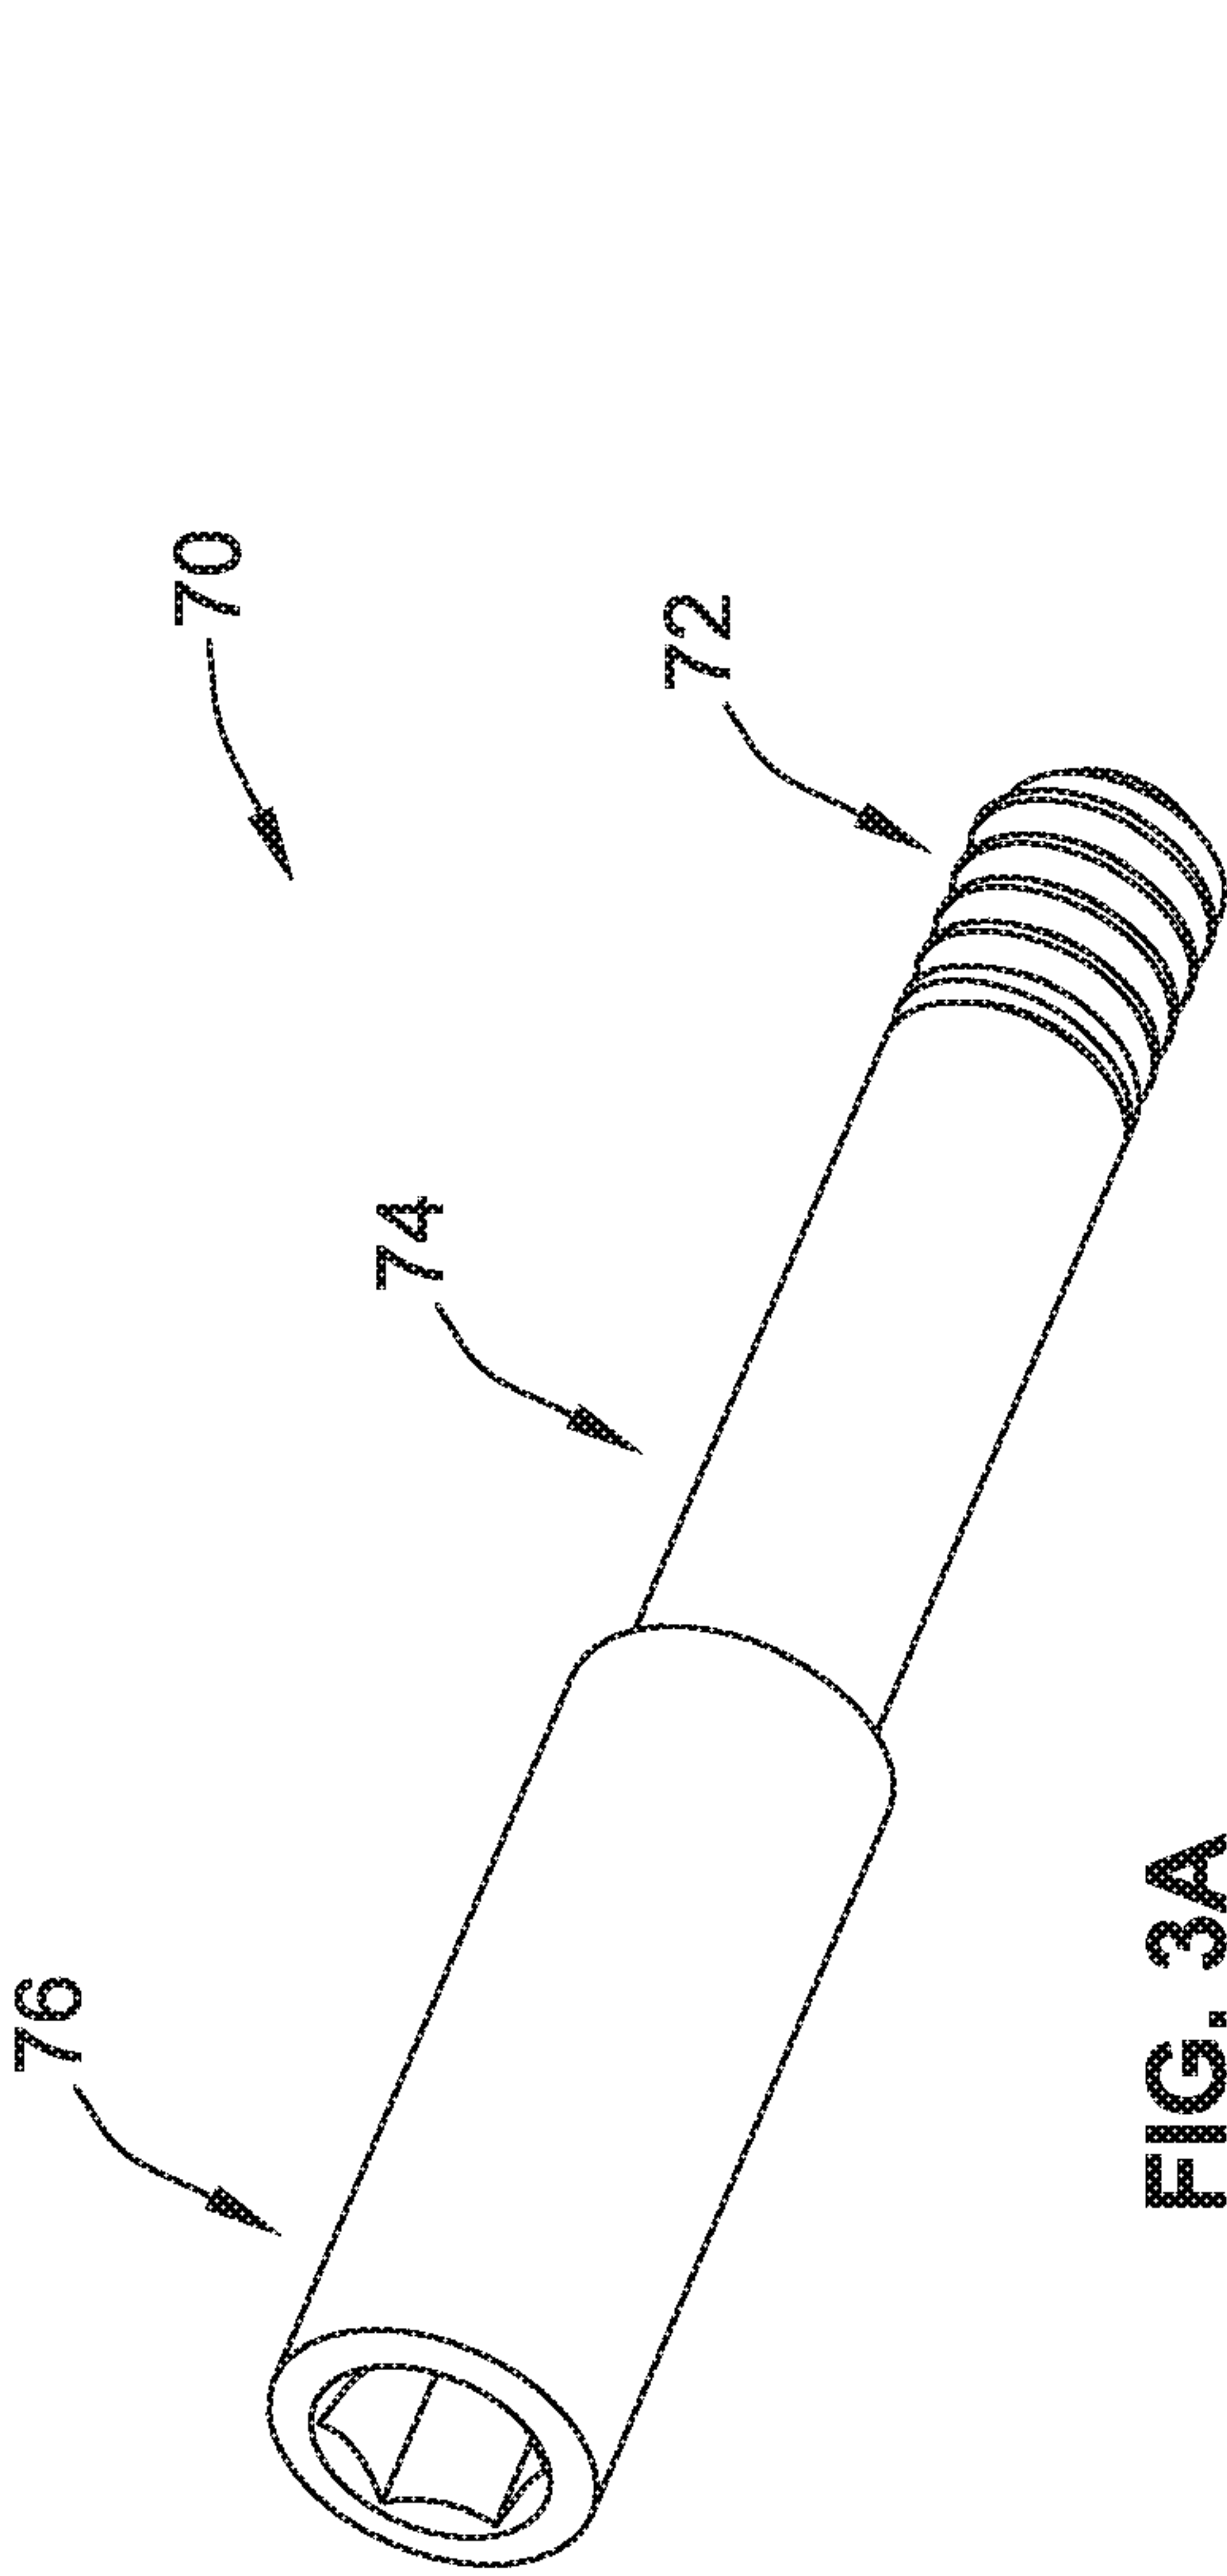


FIG. 3A

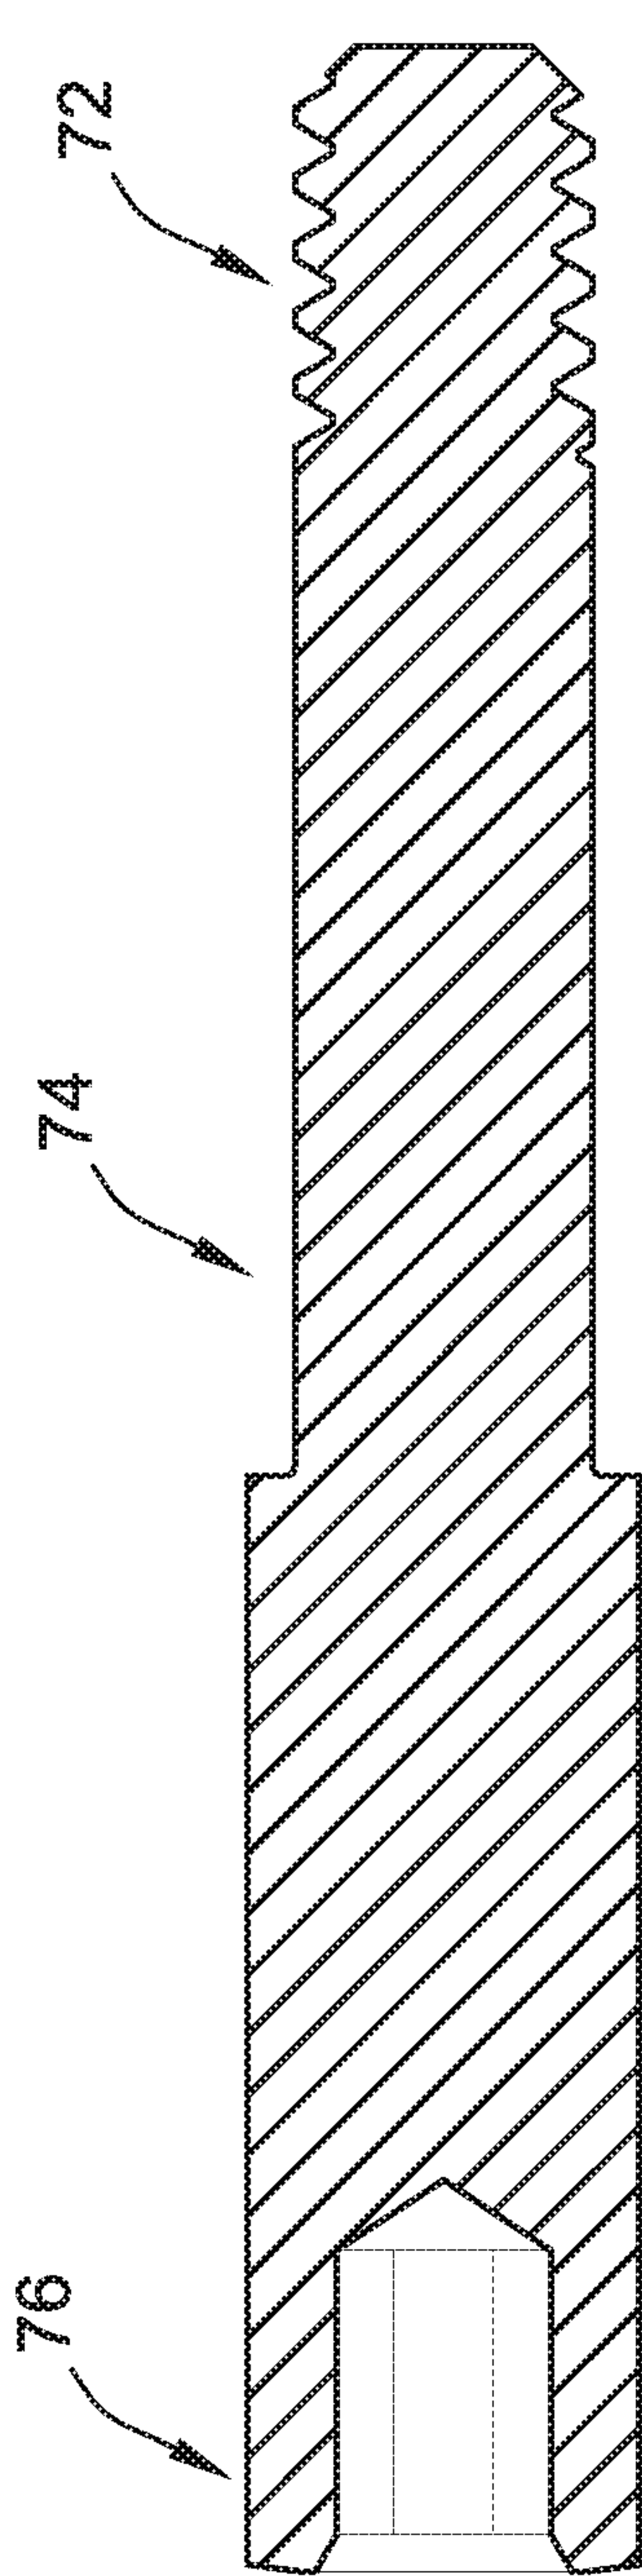


FIG. 3B



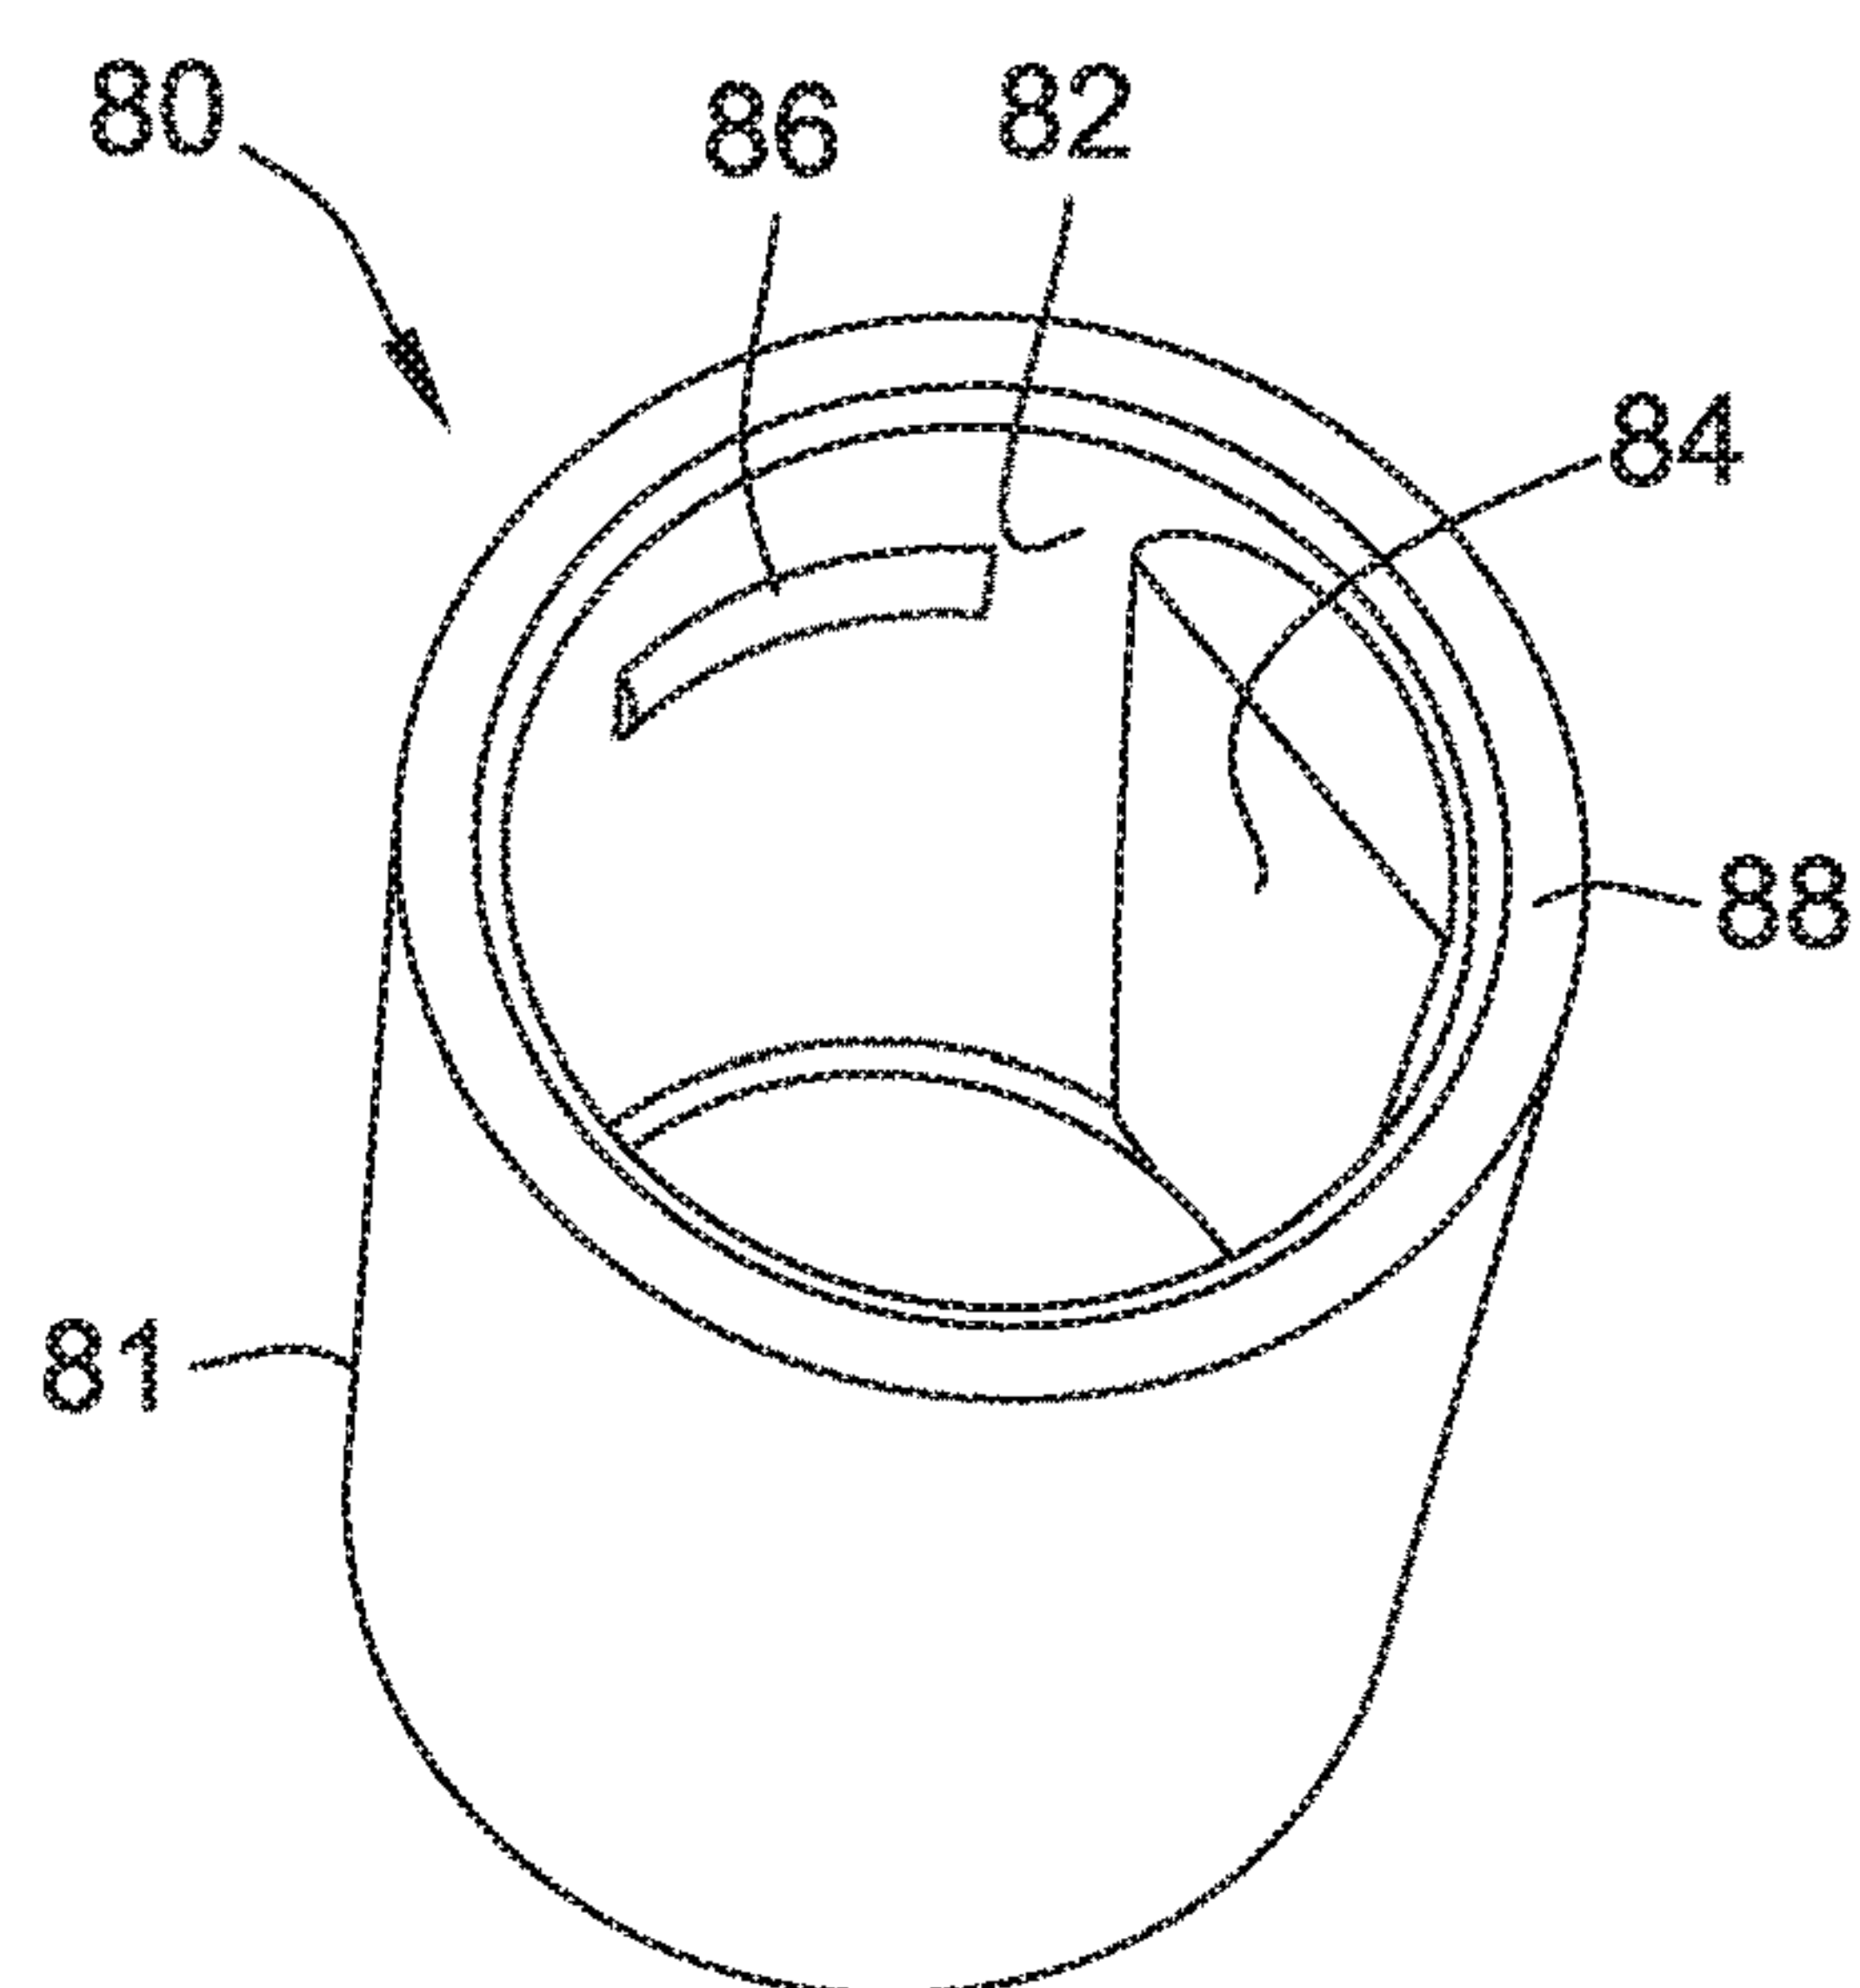


FIG. 4A

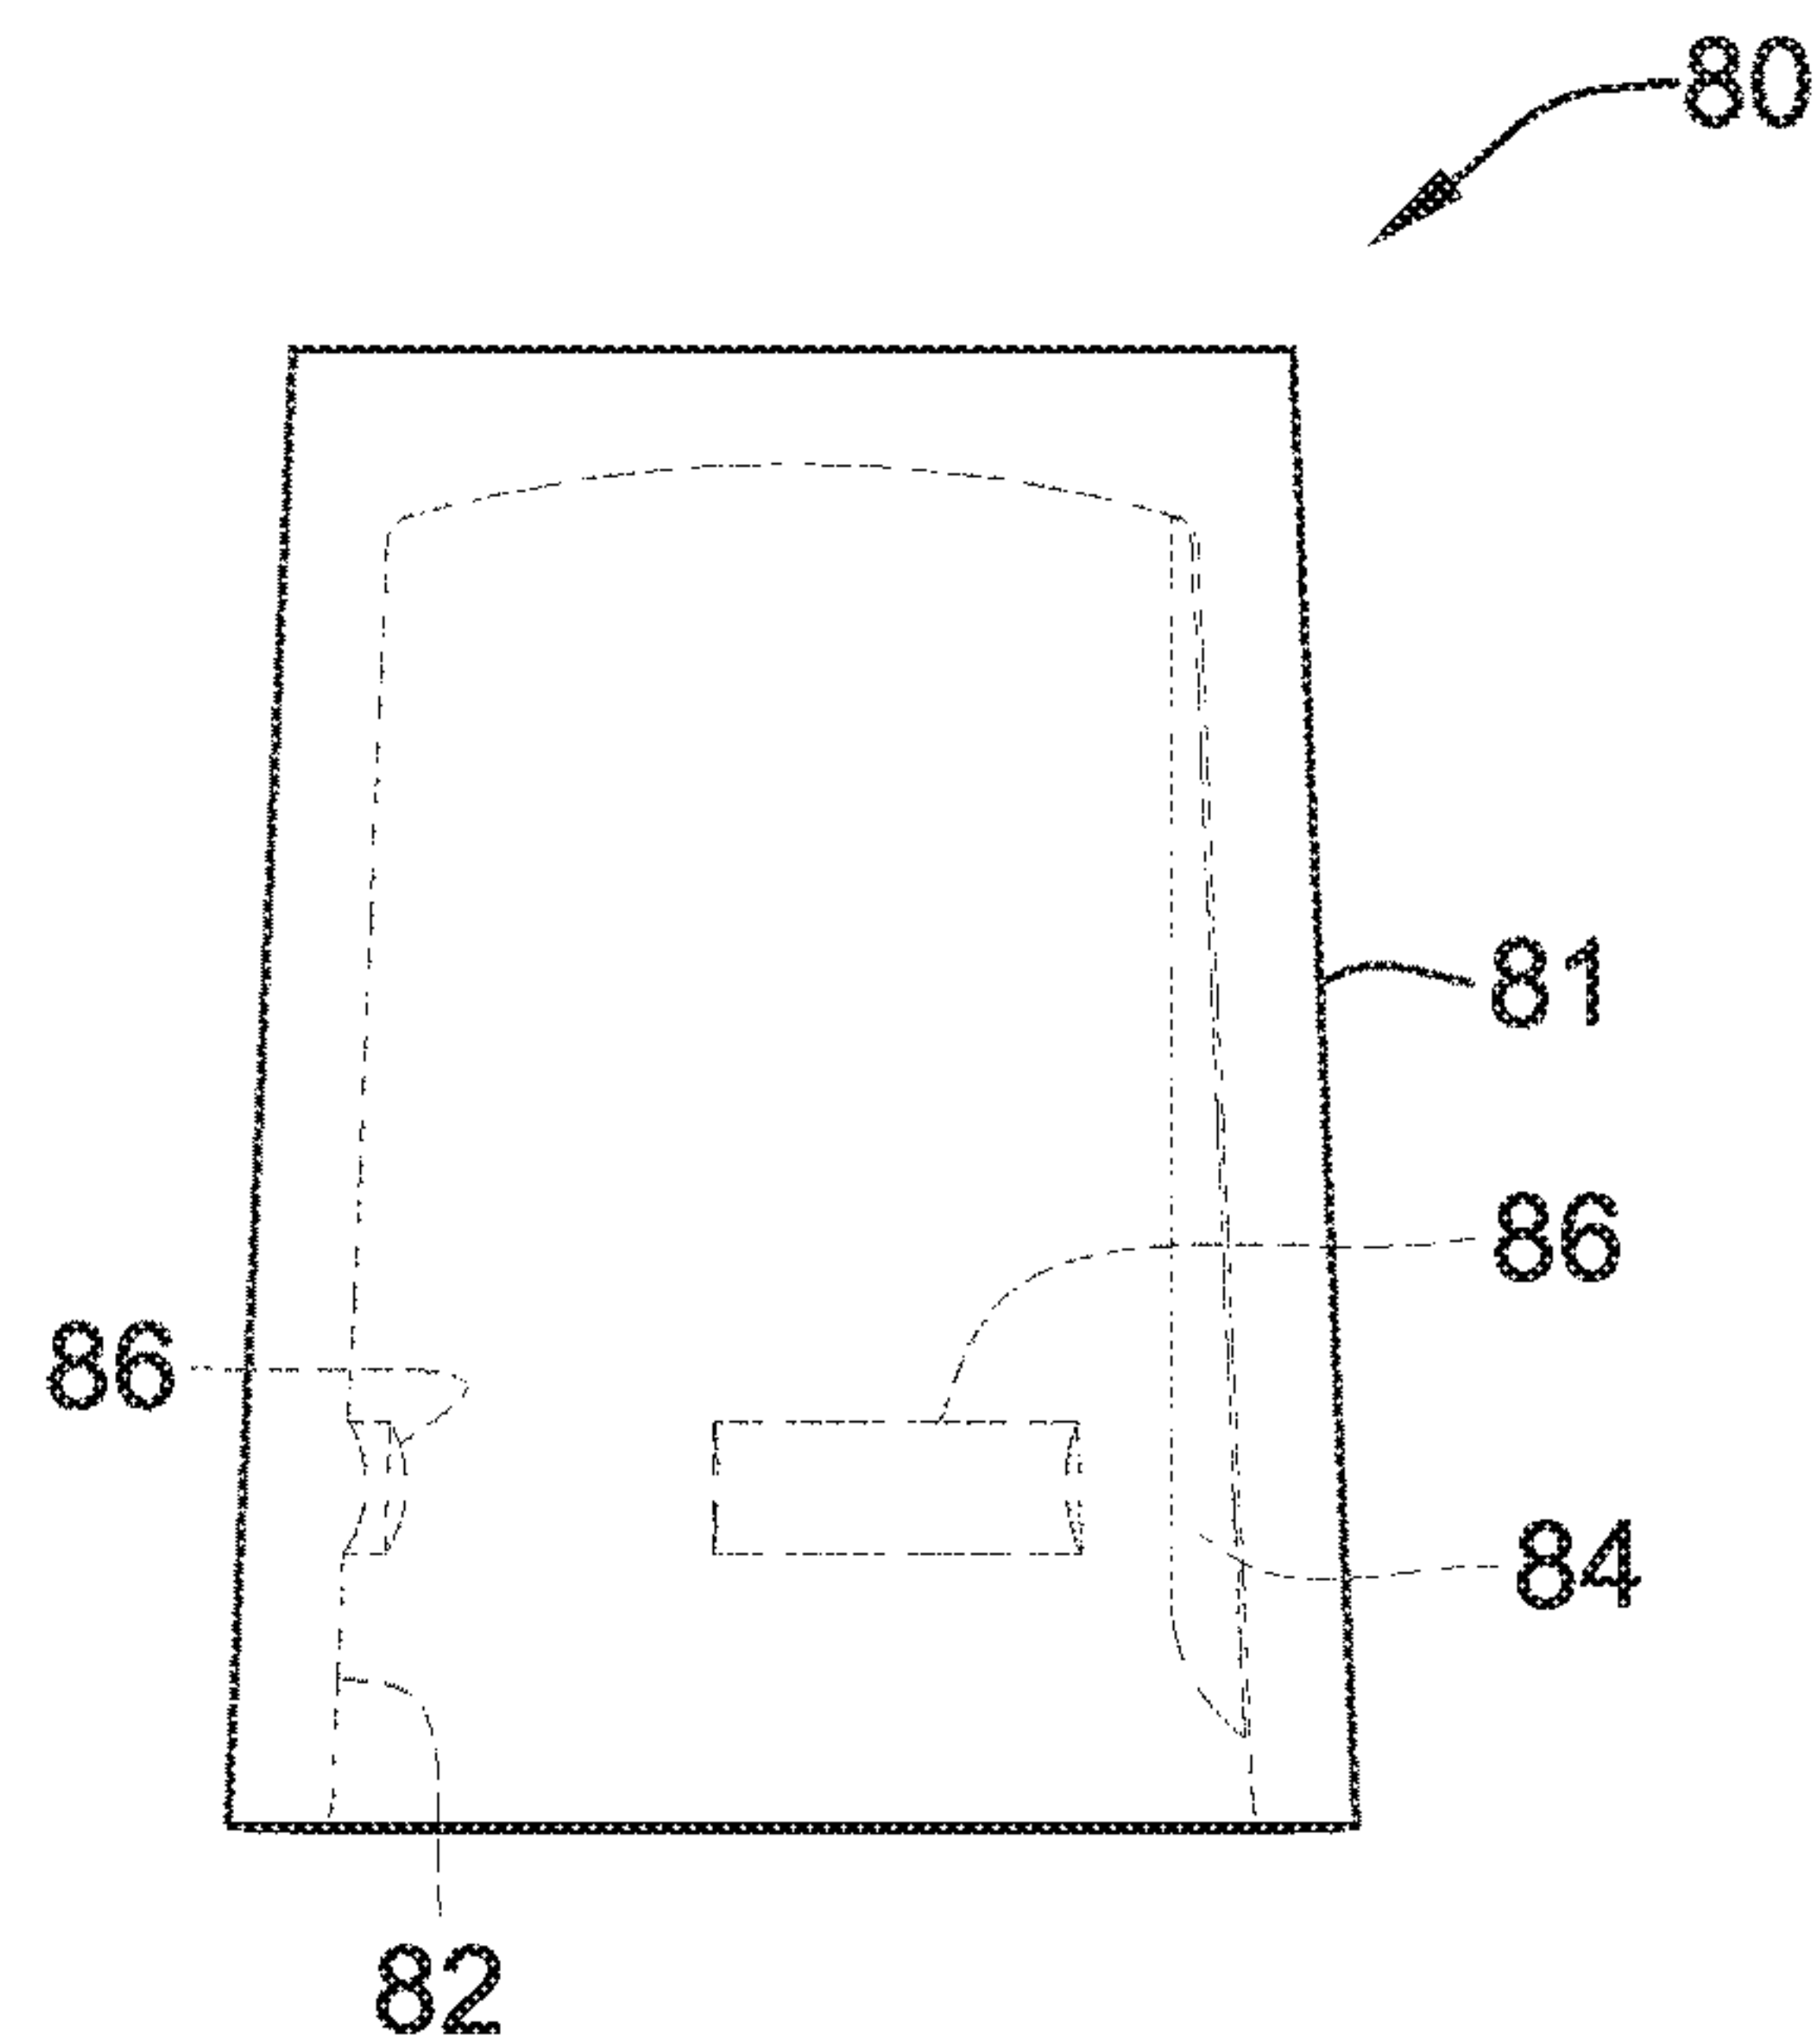


FIG. 4B

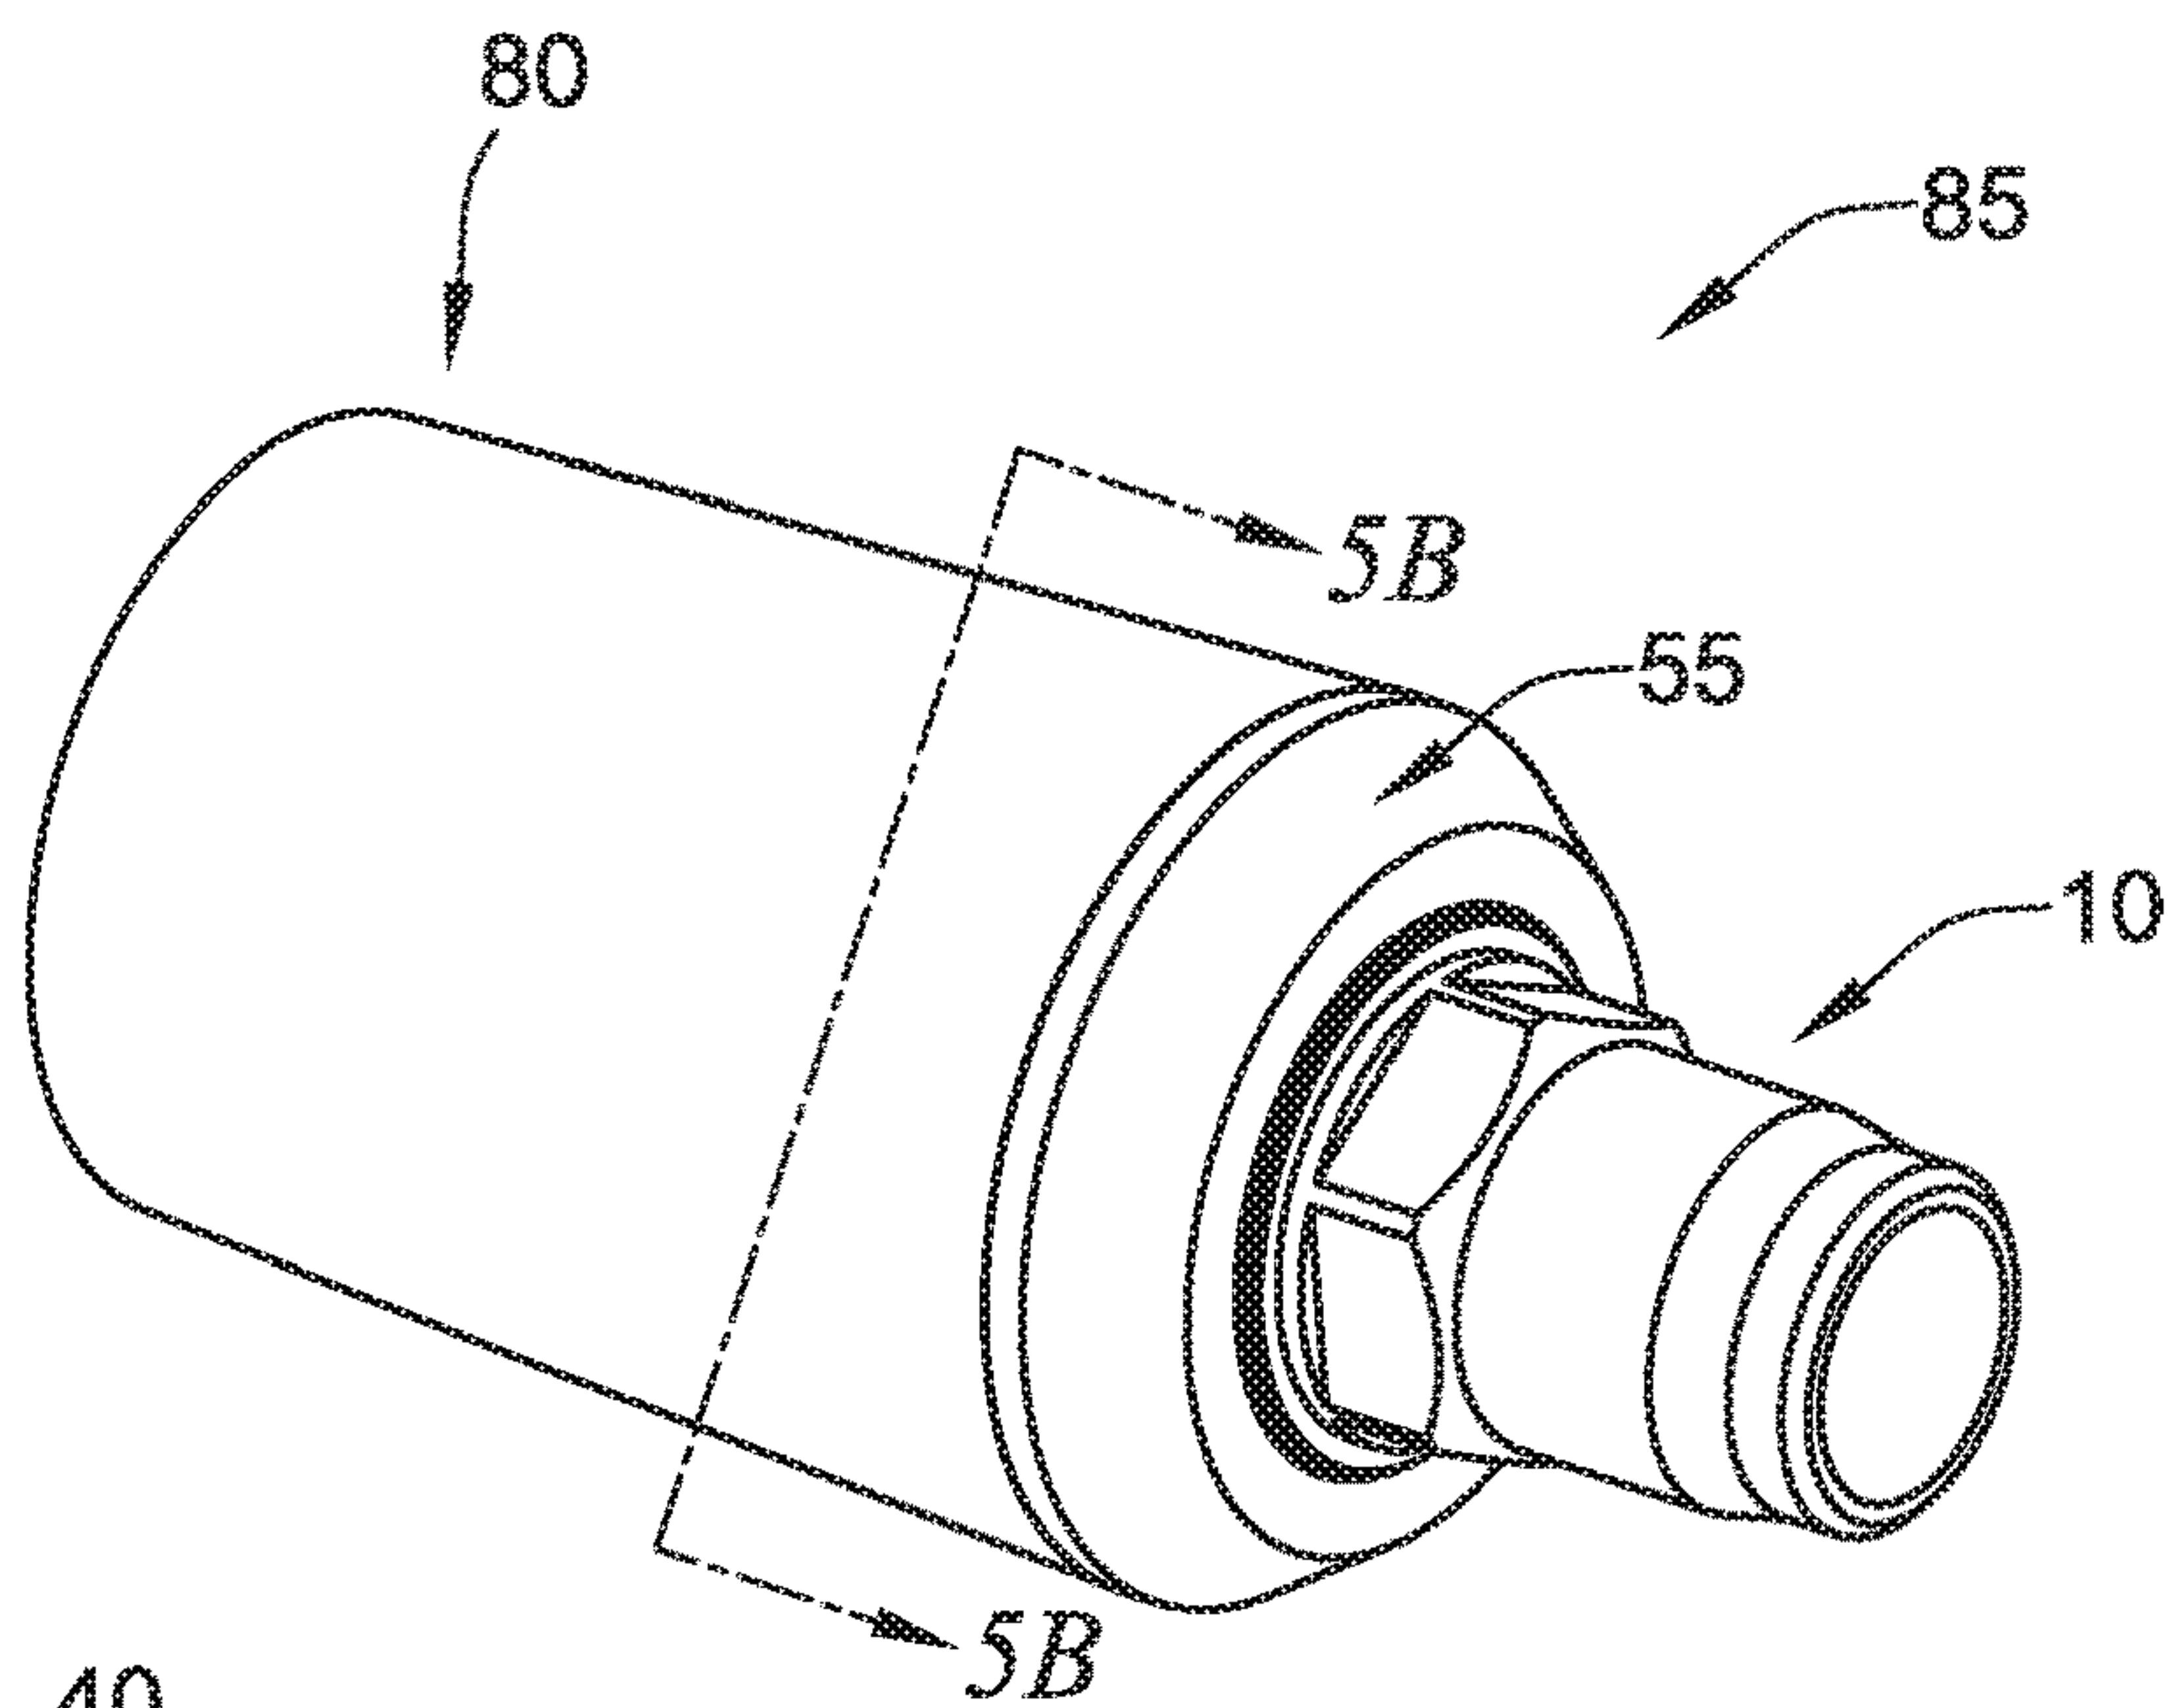


FIG. 5A

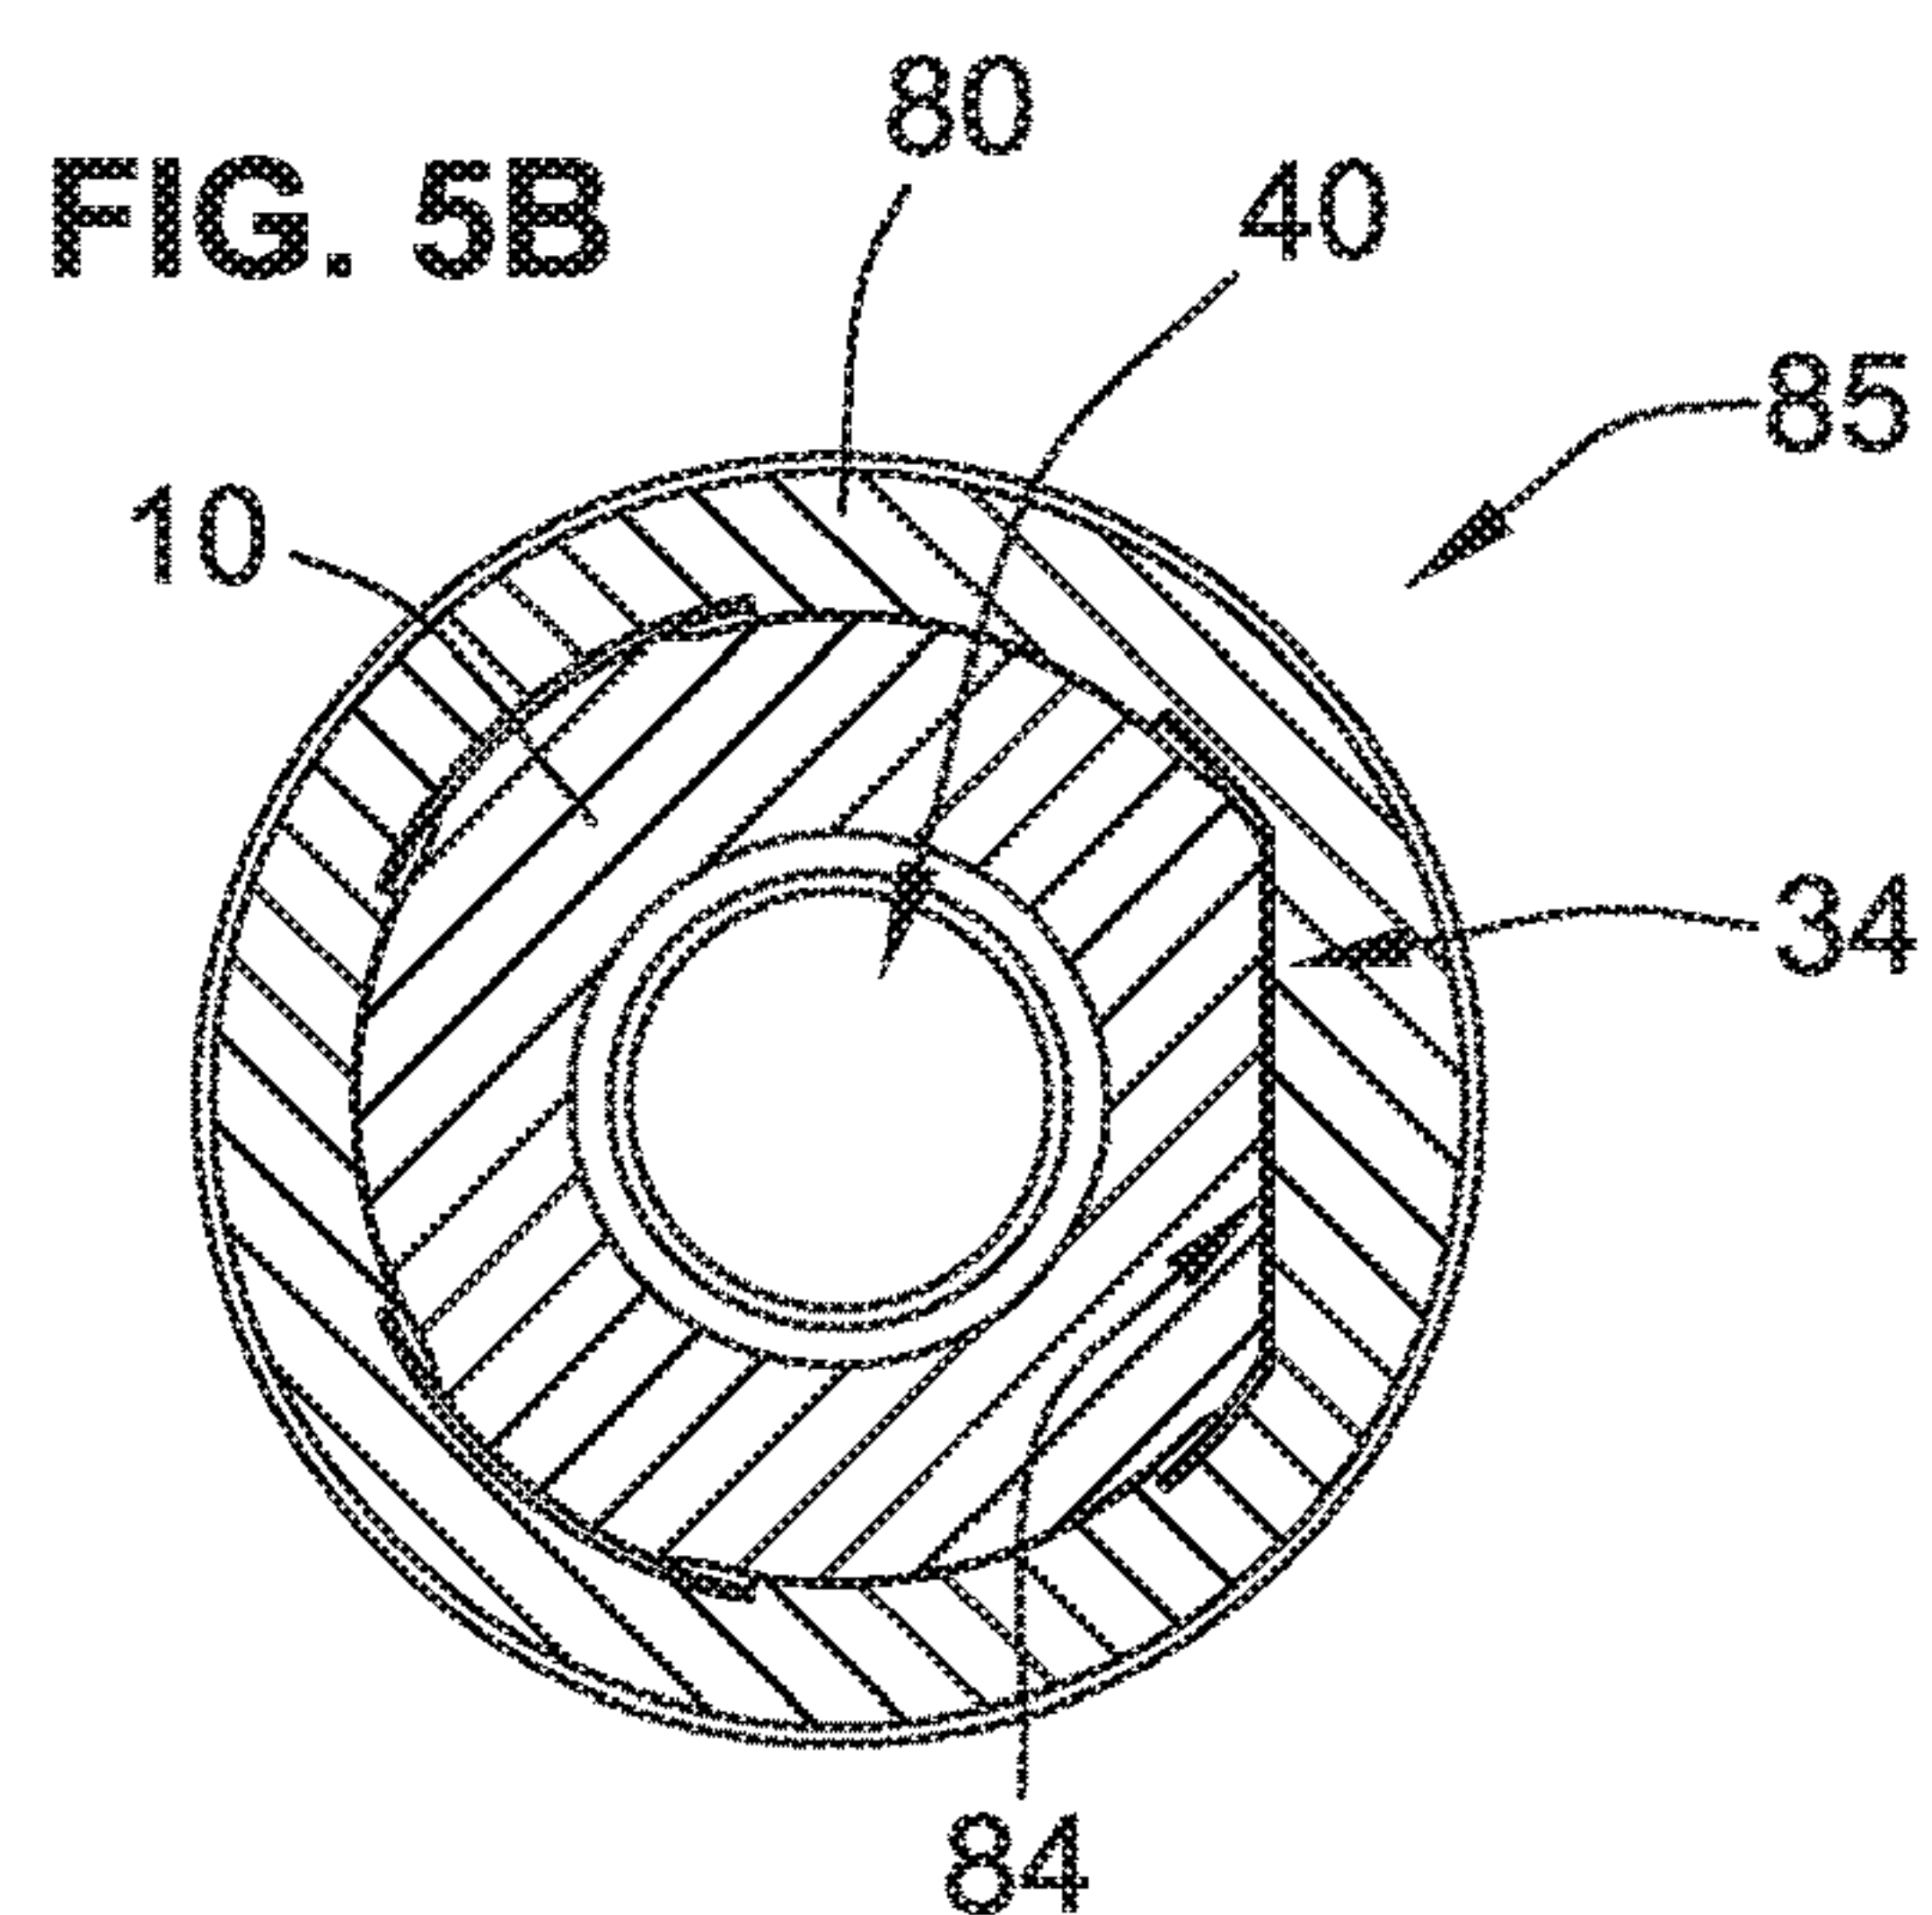
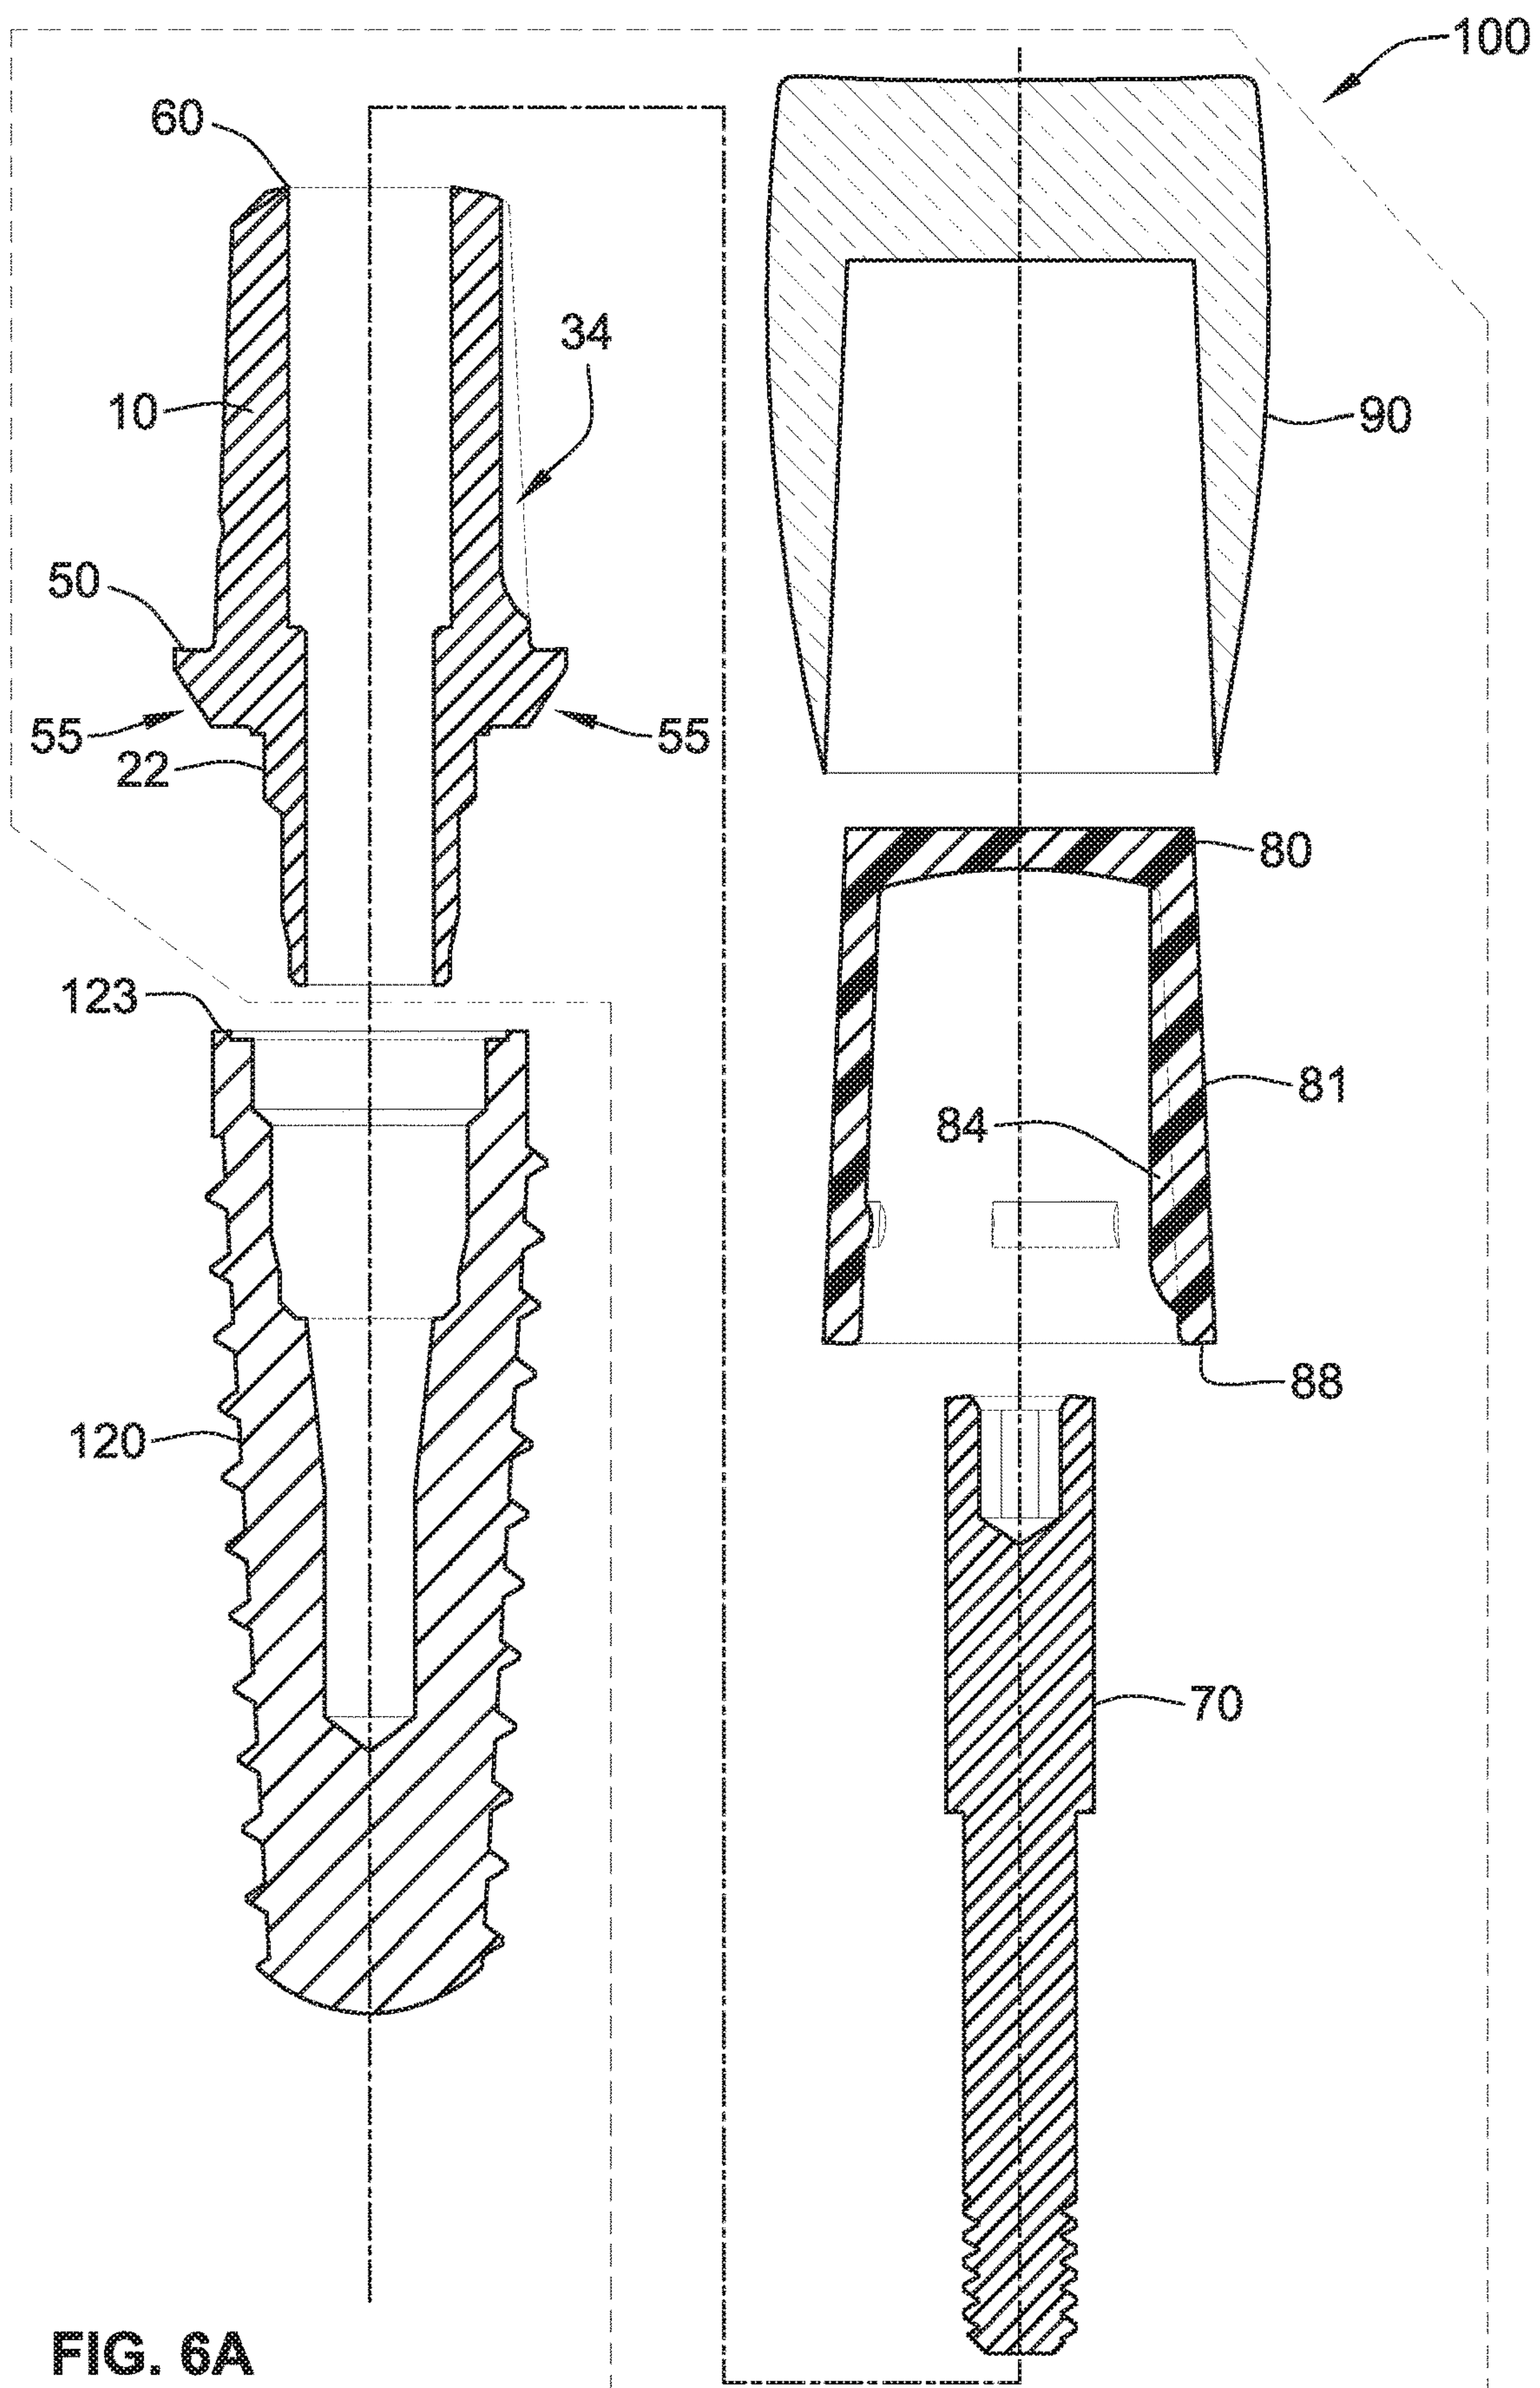


FIG. 5B





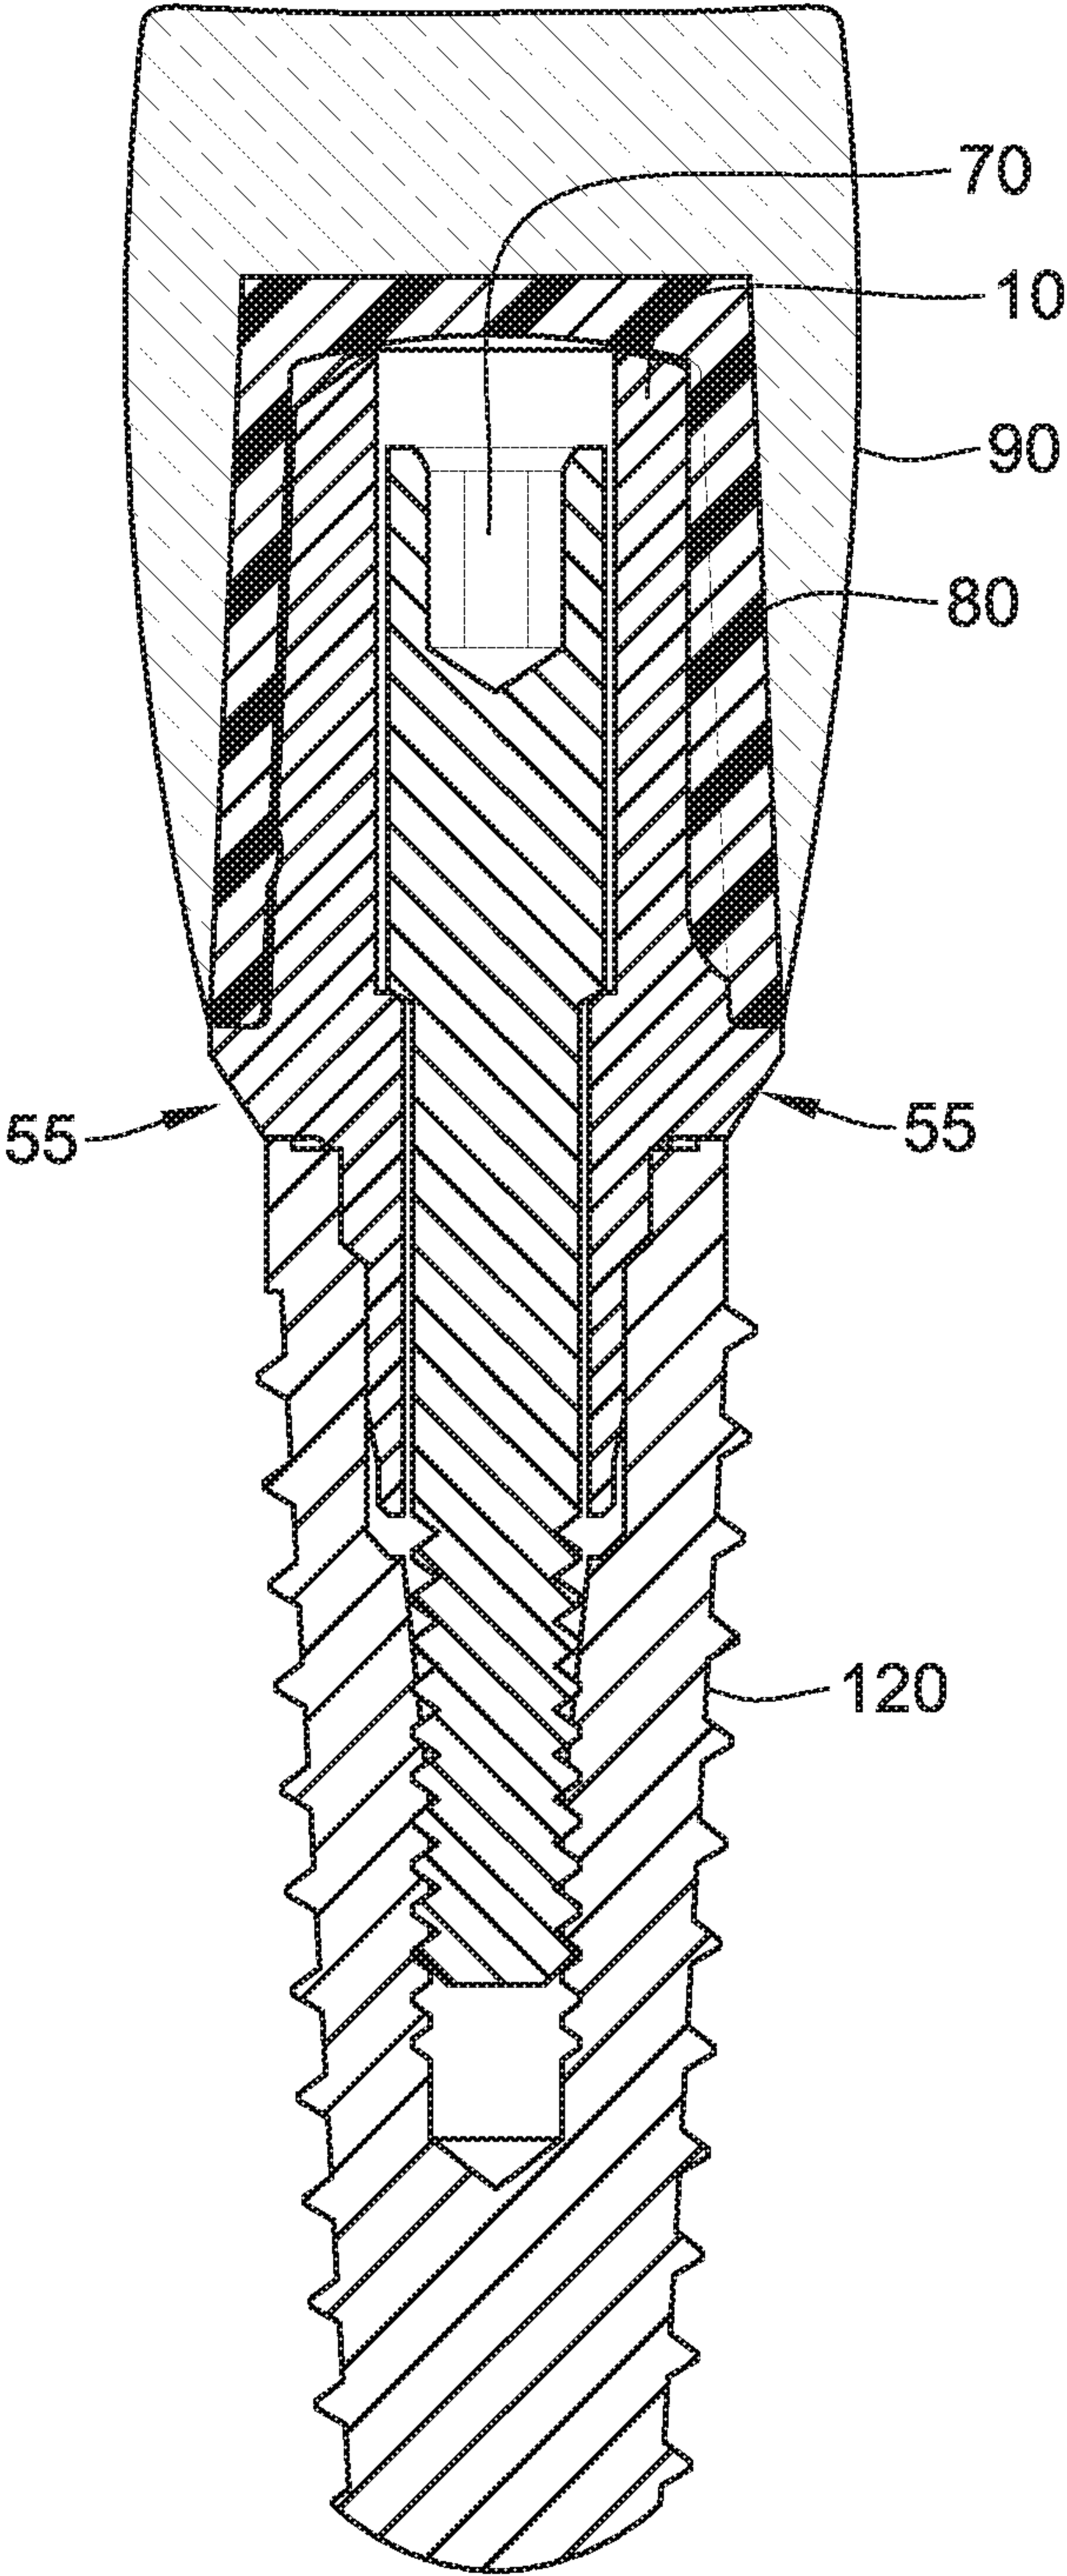


FIG. 6B

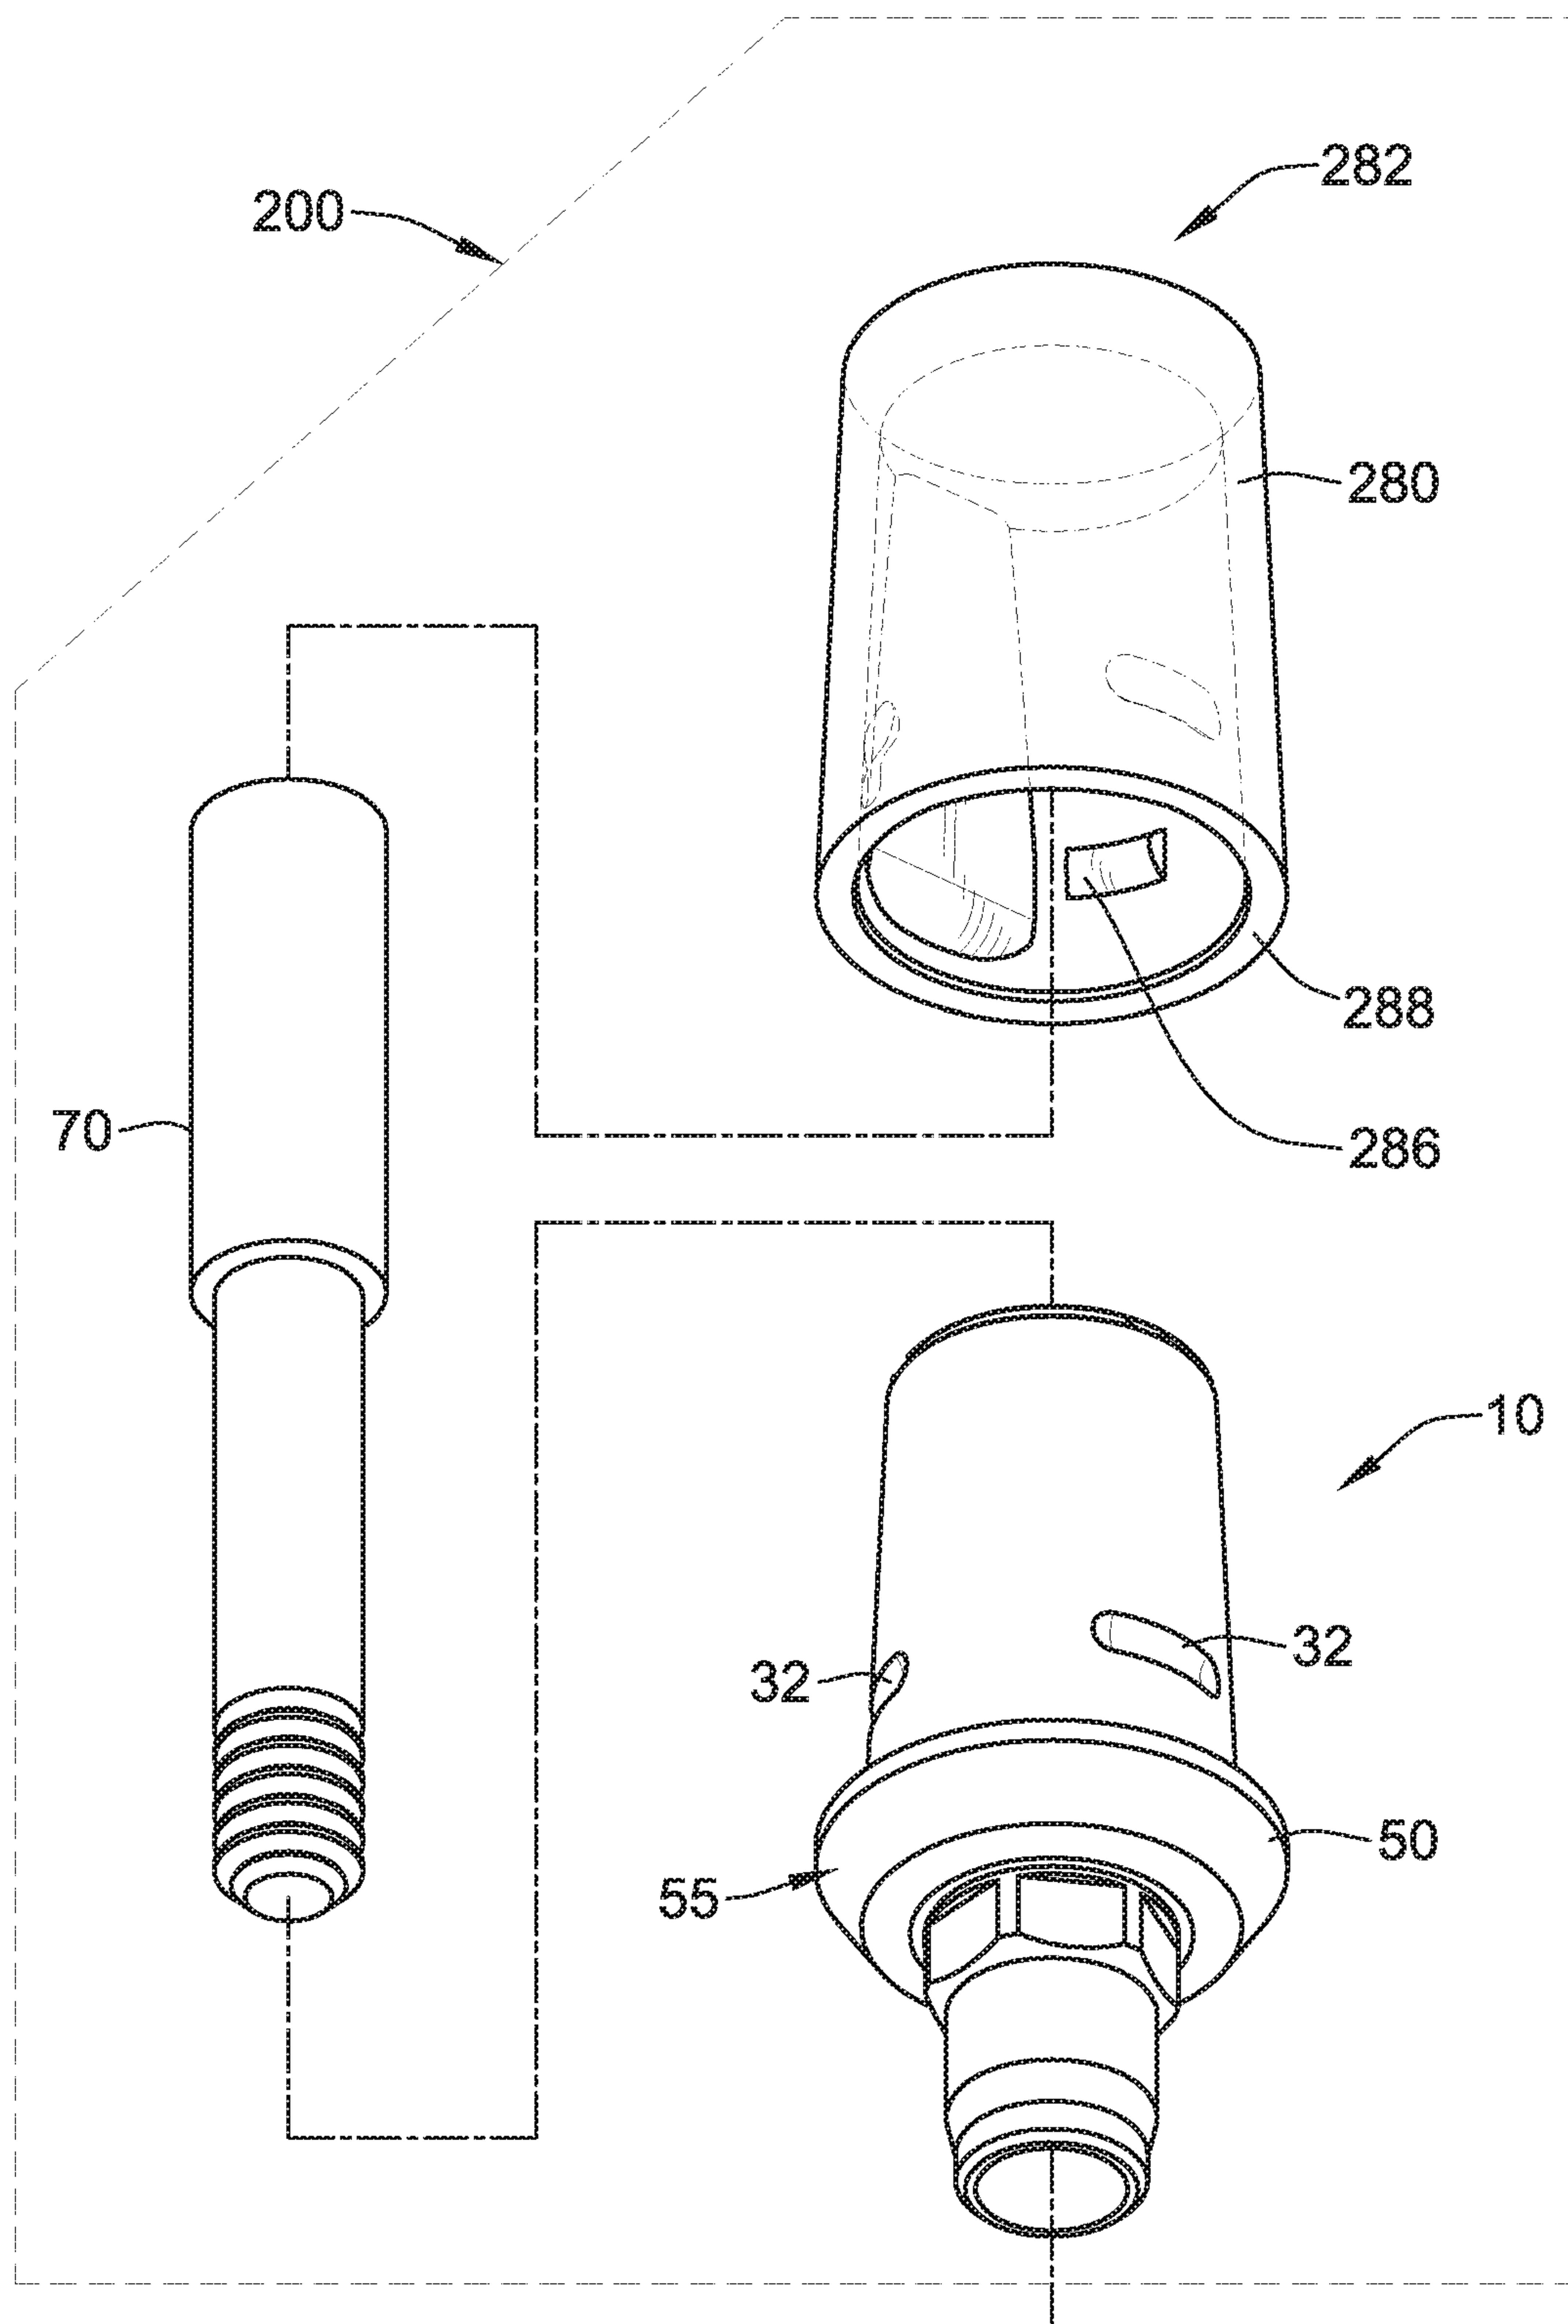


FIG. 7A



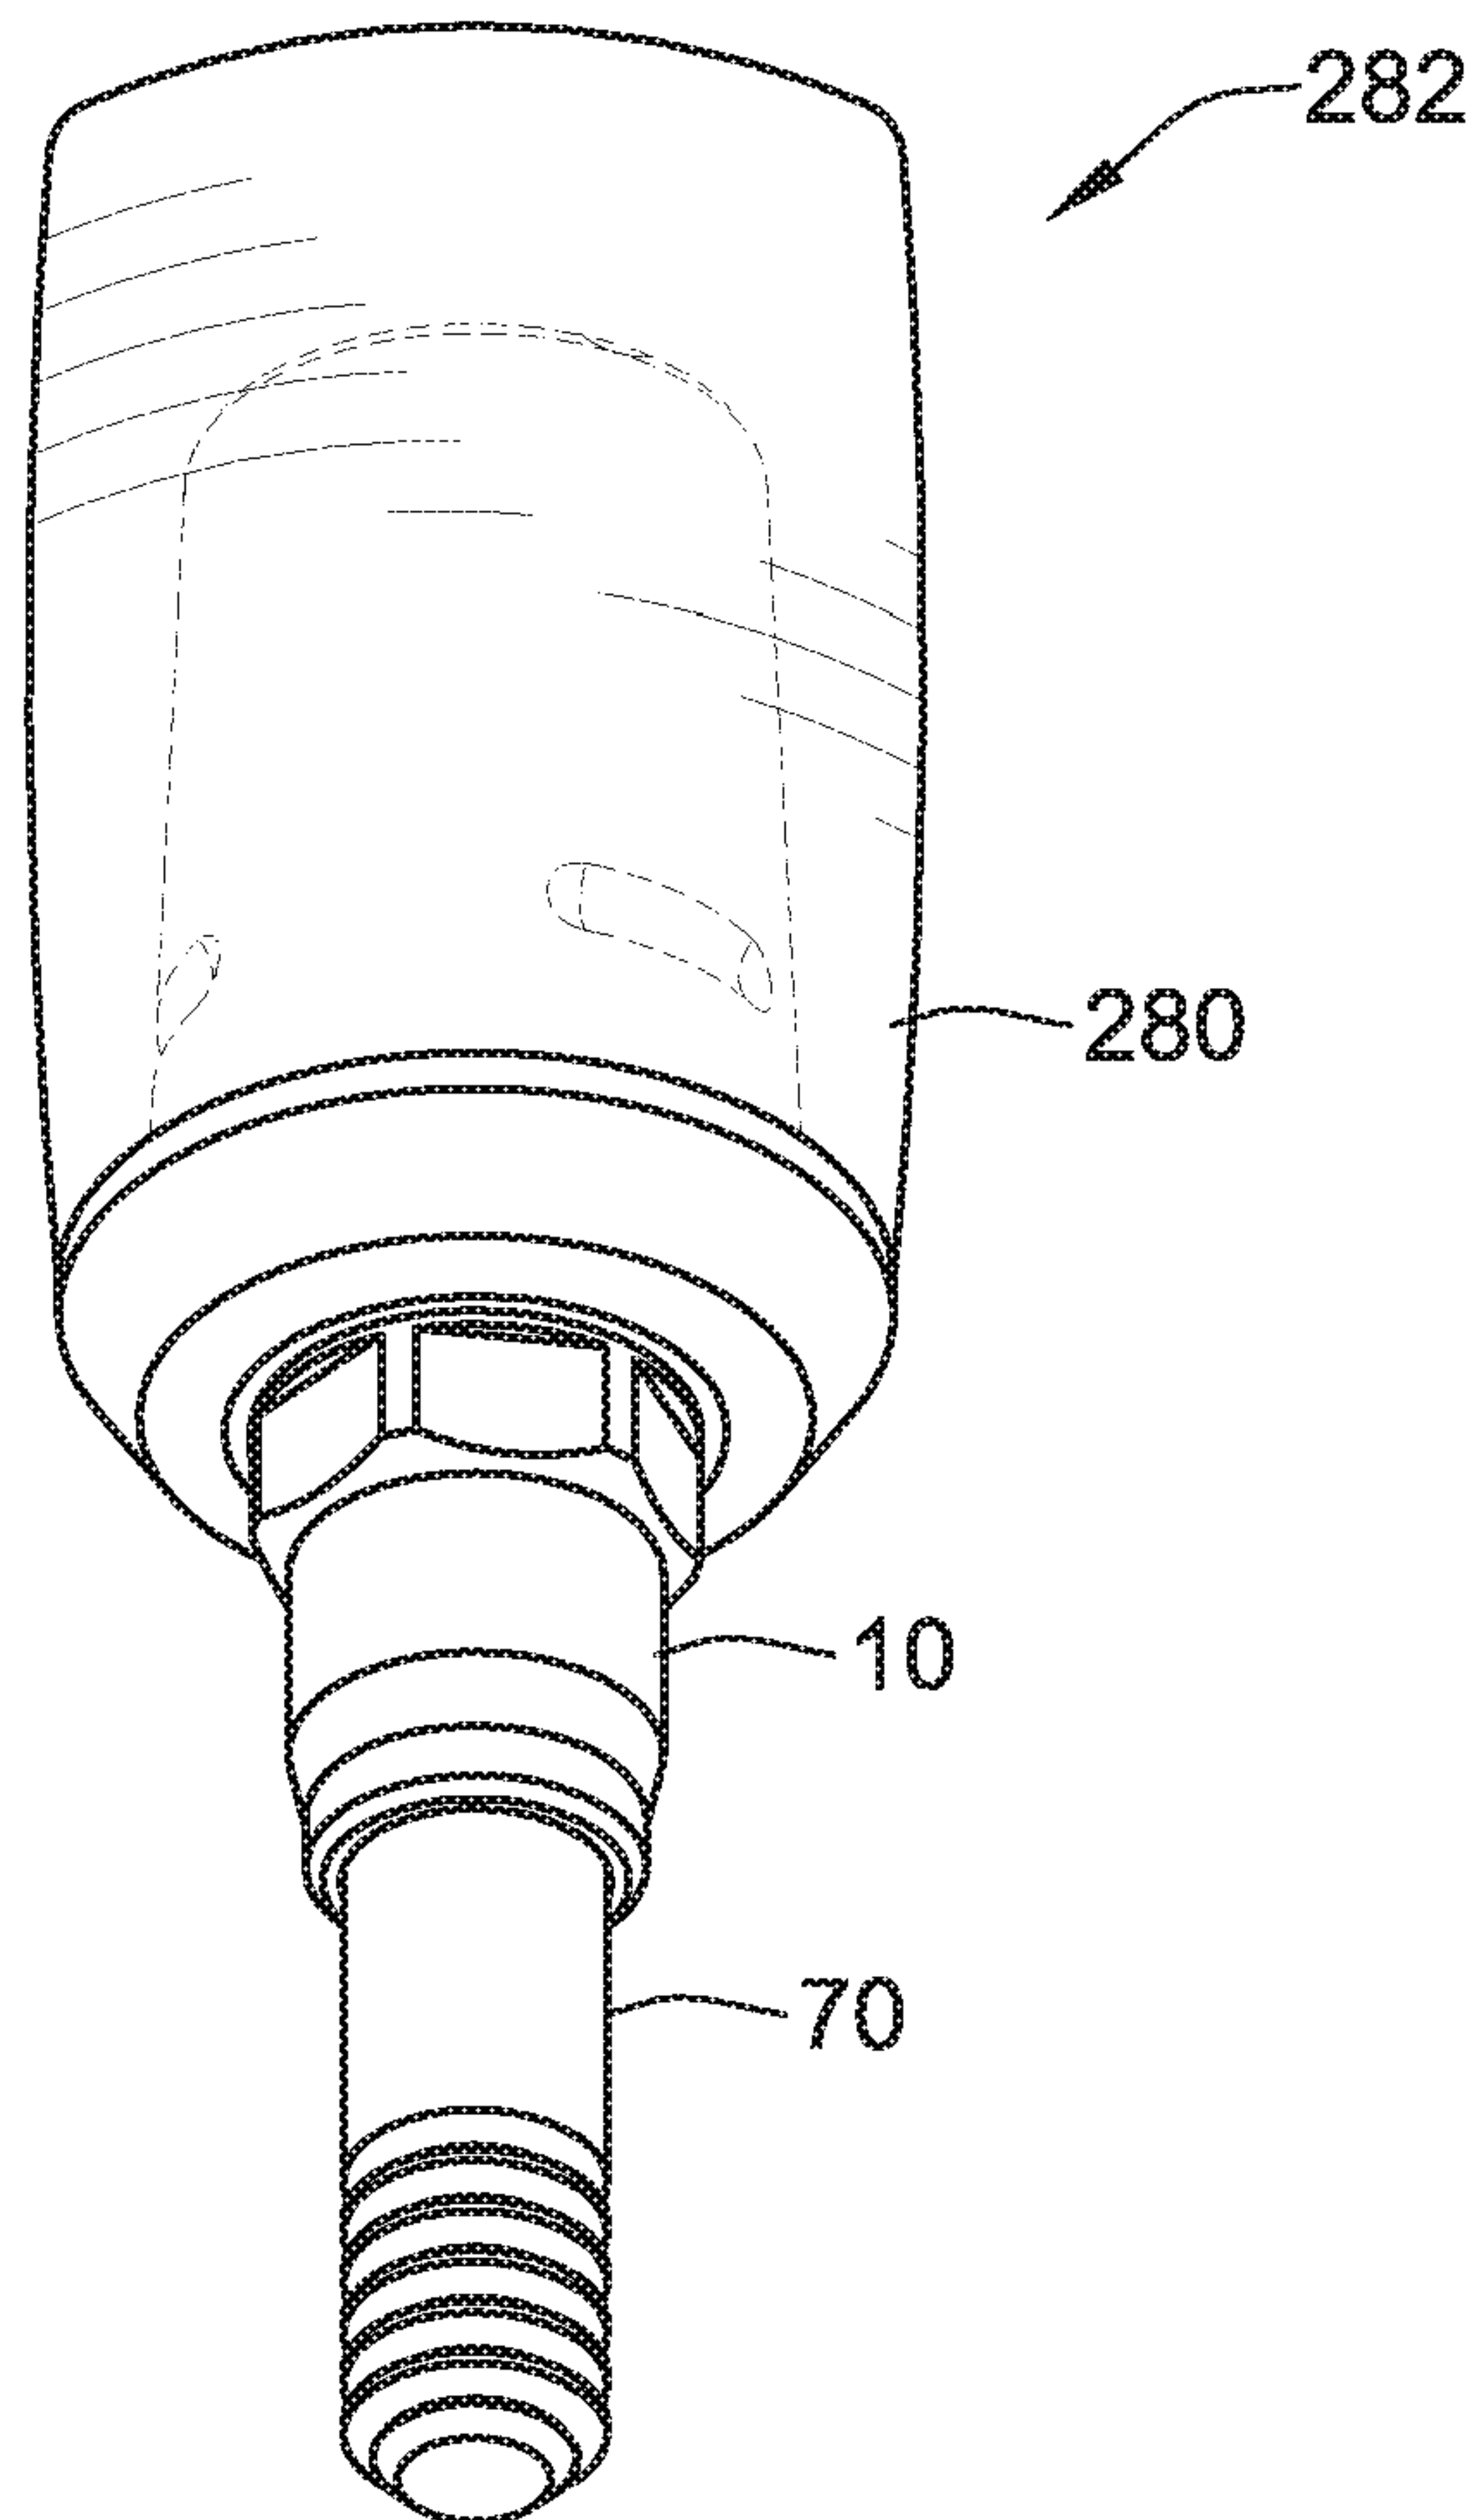


FIG. 7B

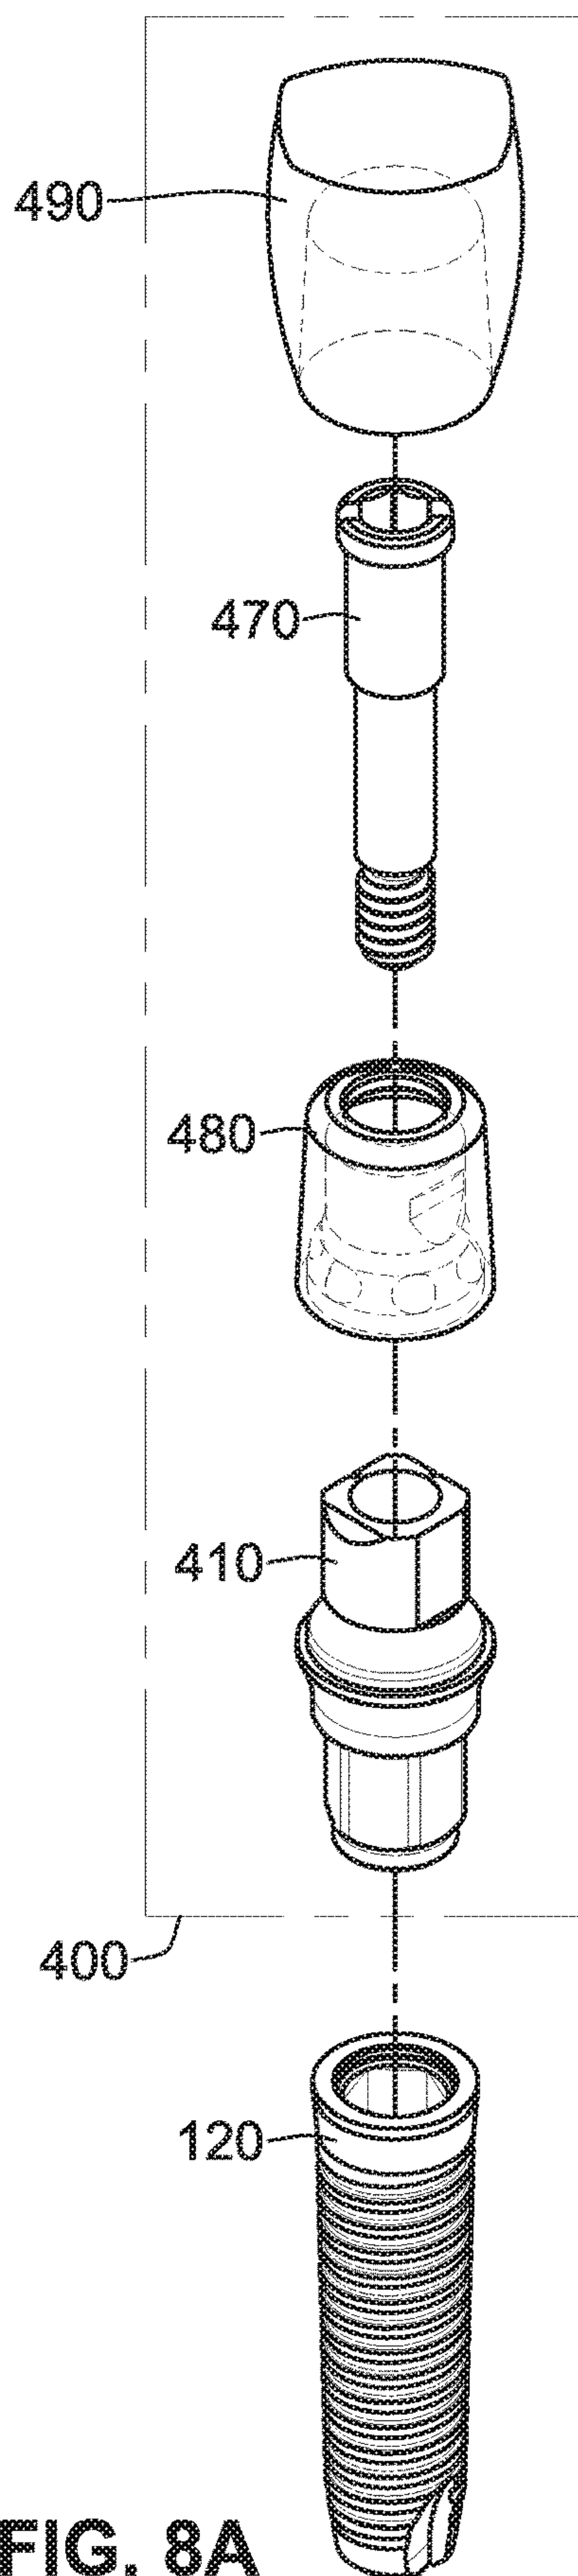


FIG. 8A

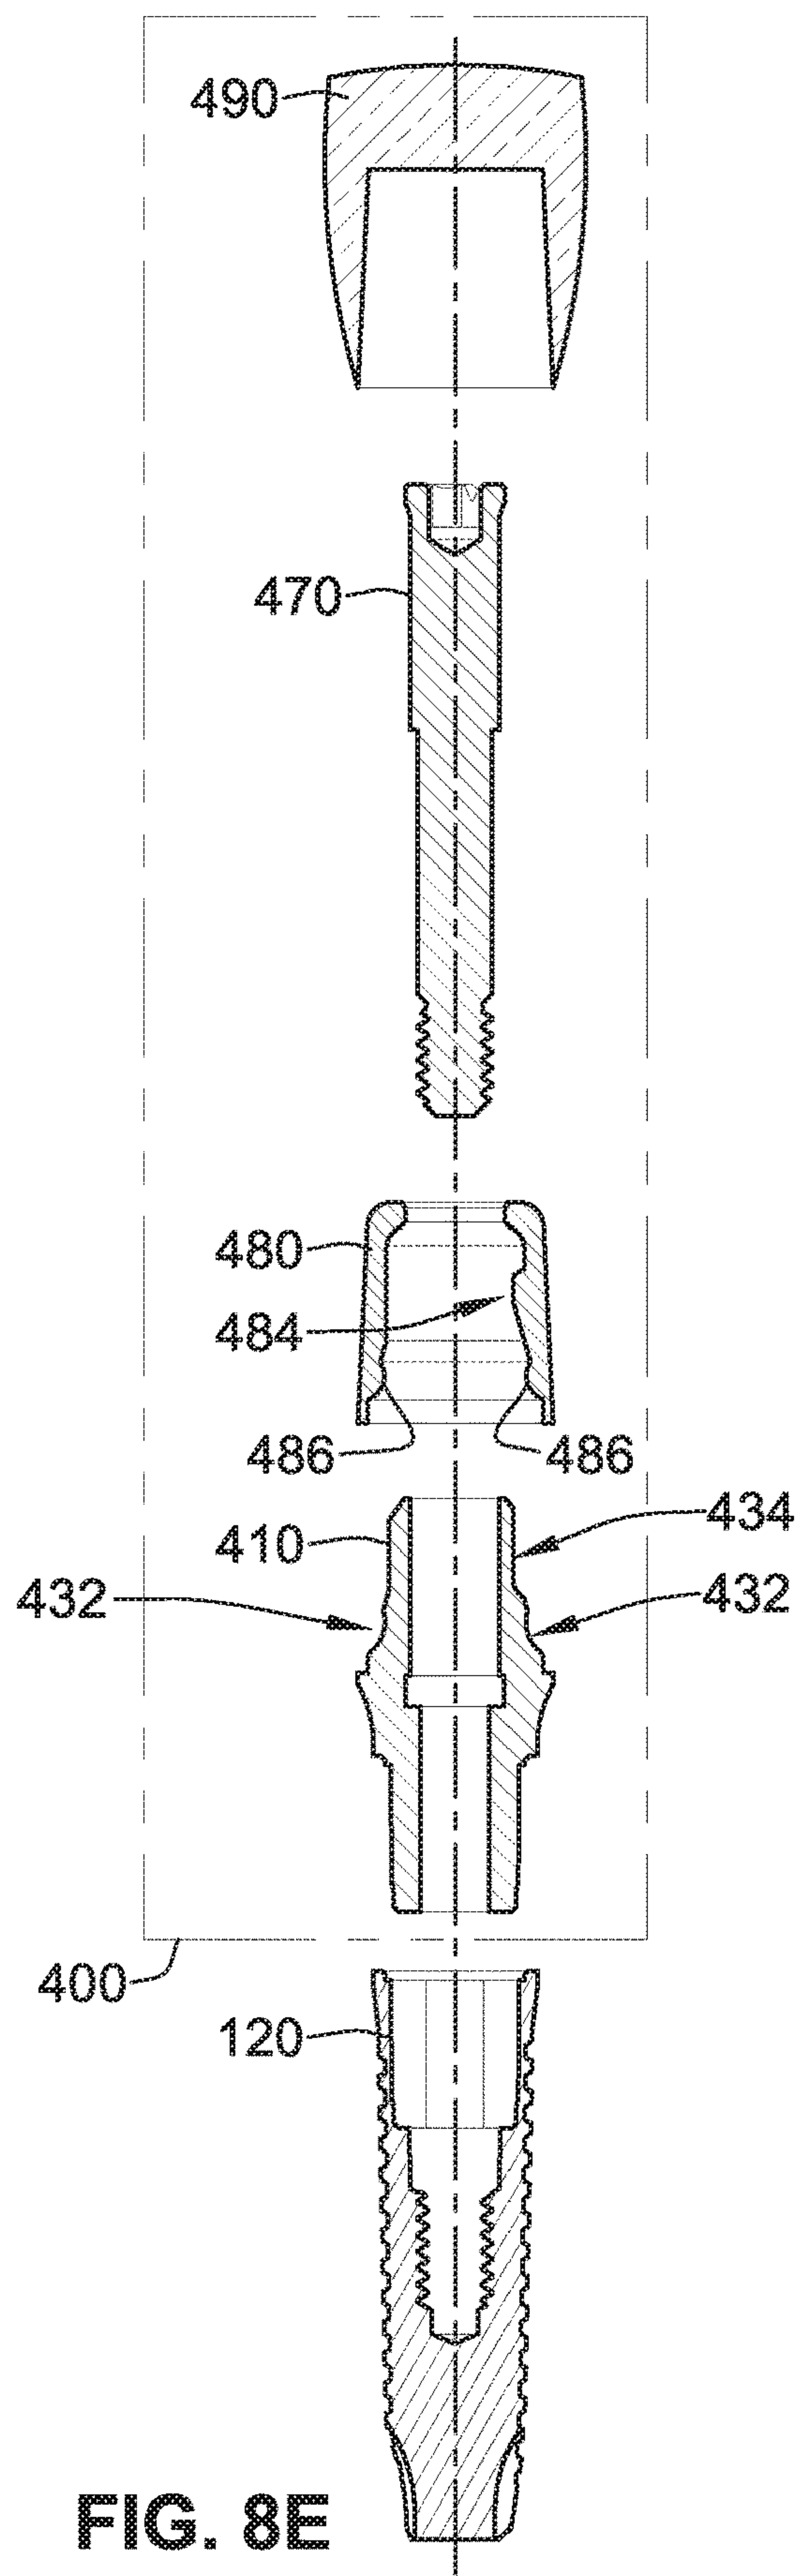
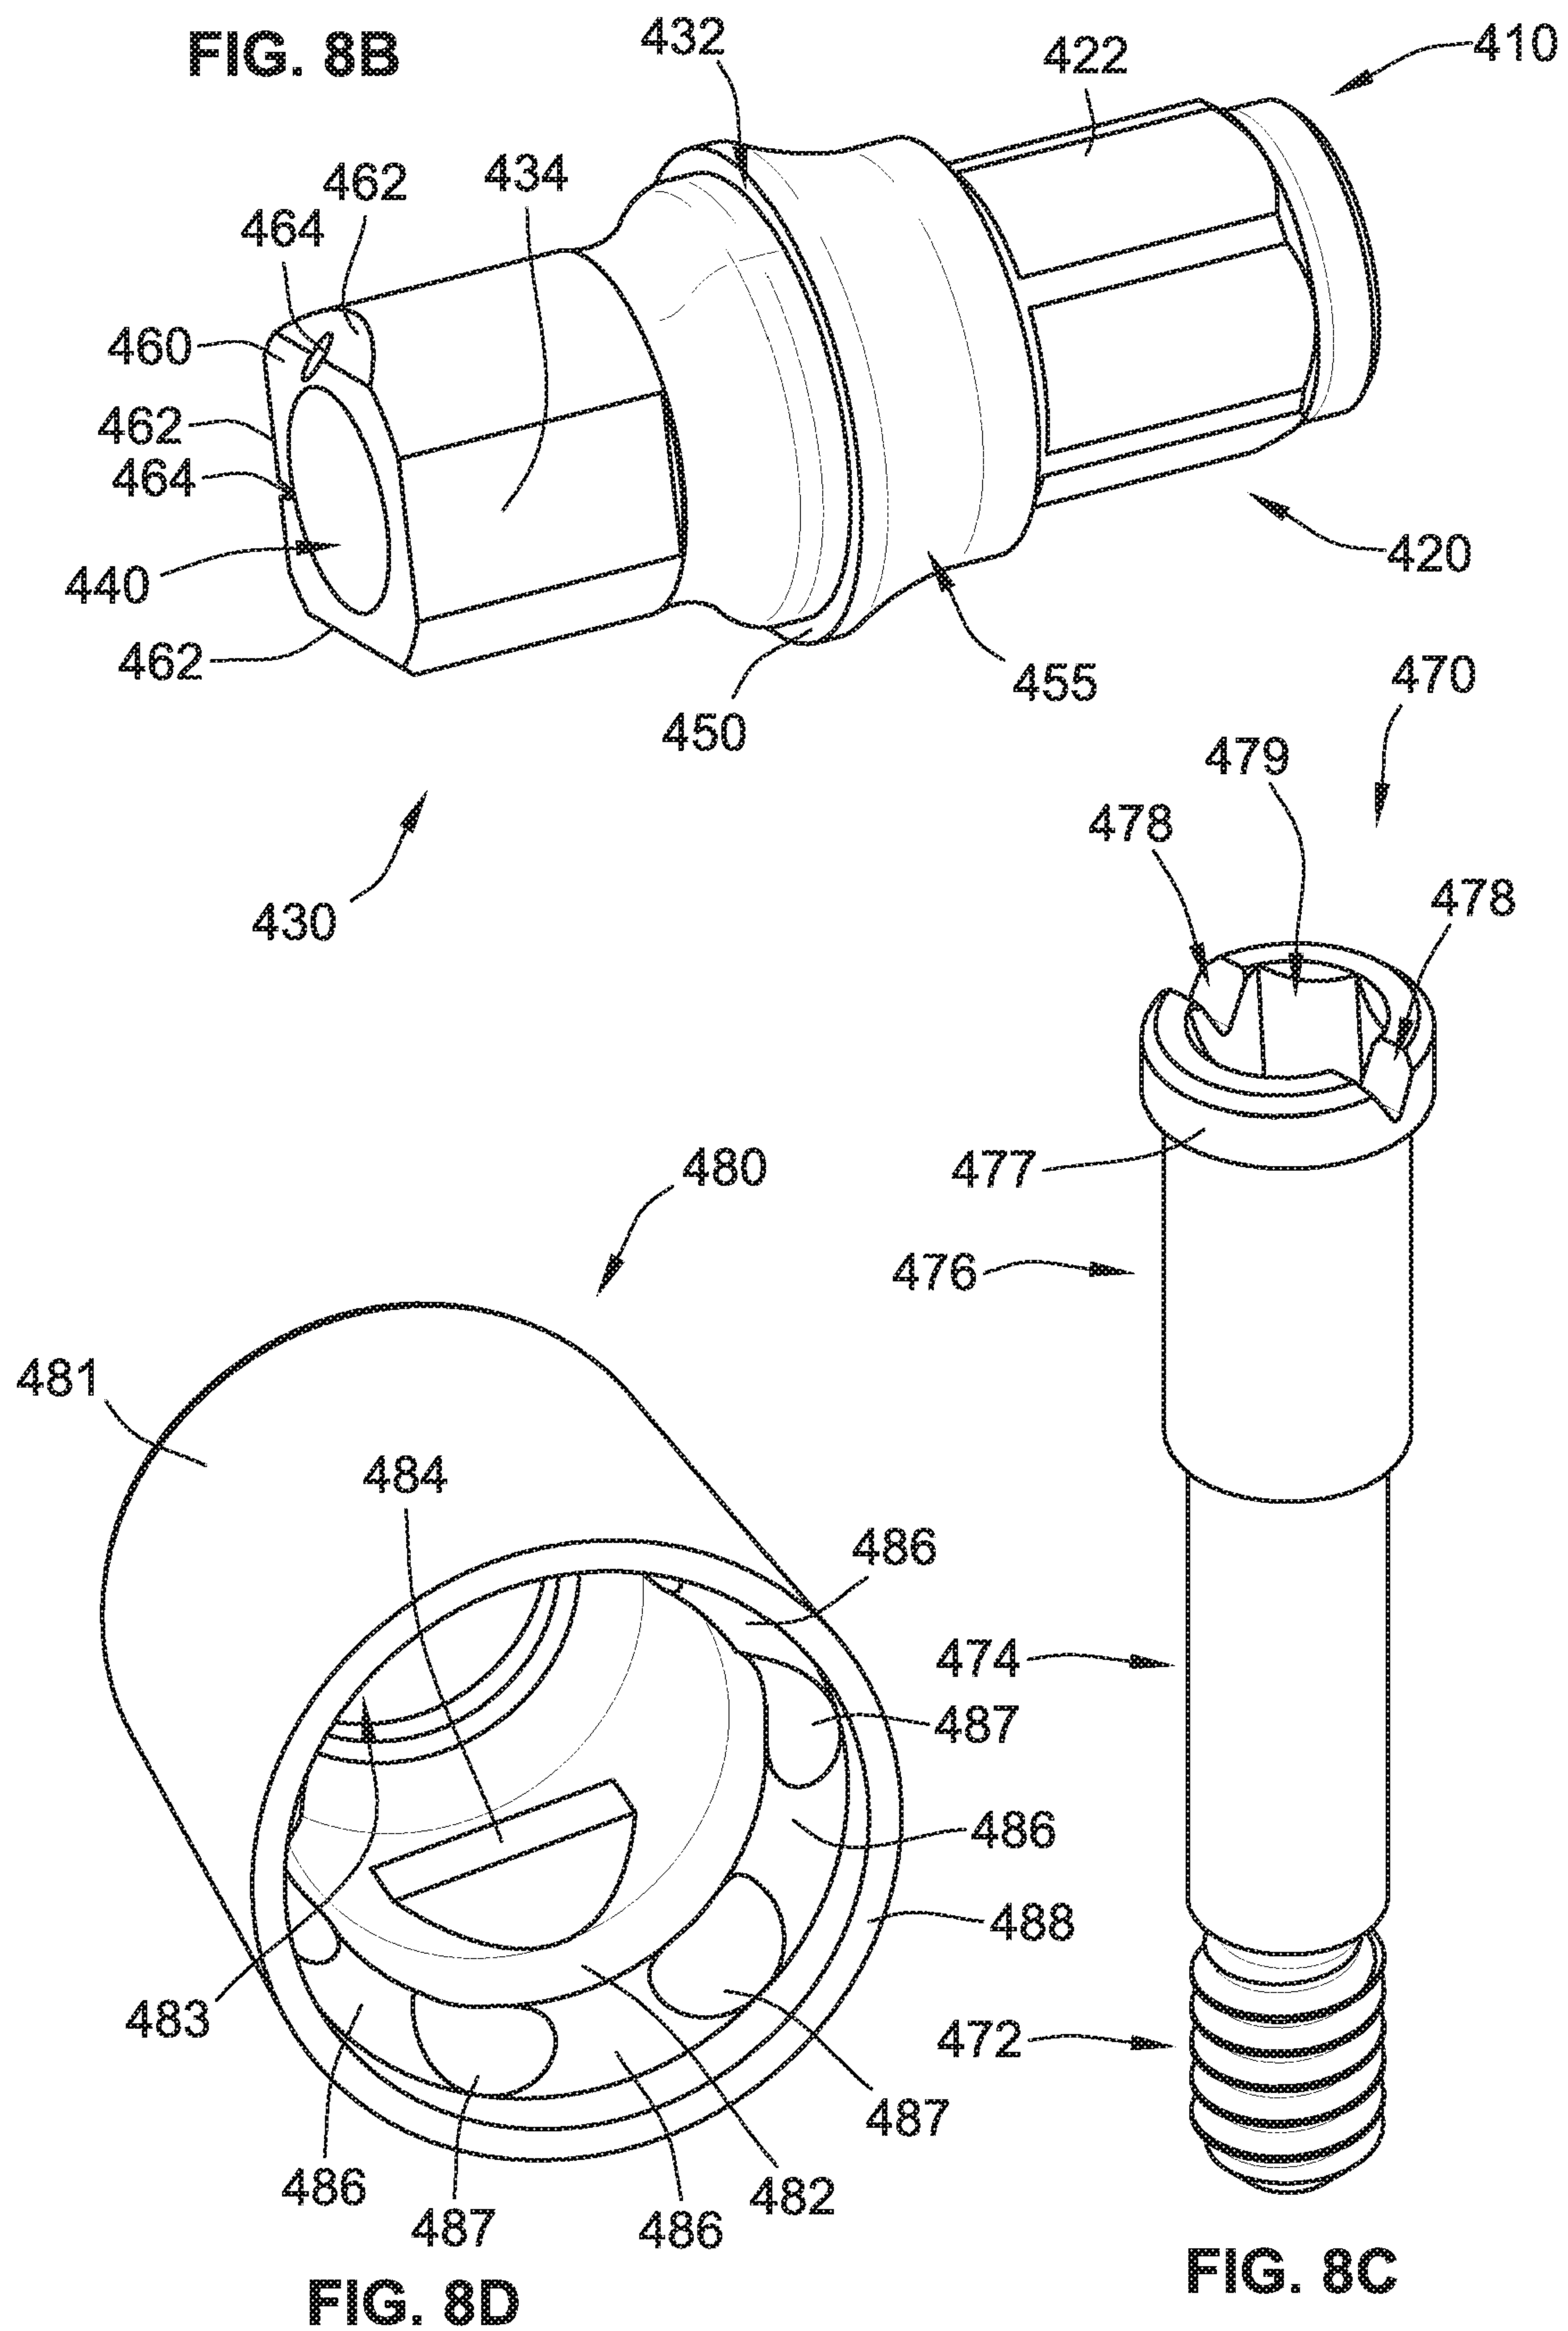


FIG. 8E





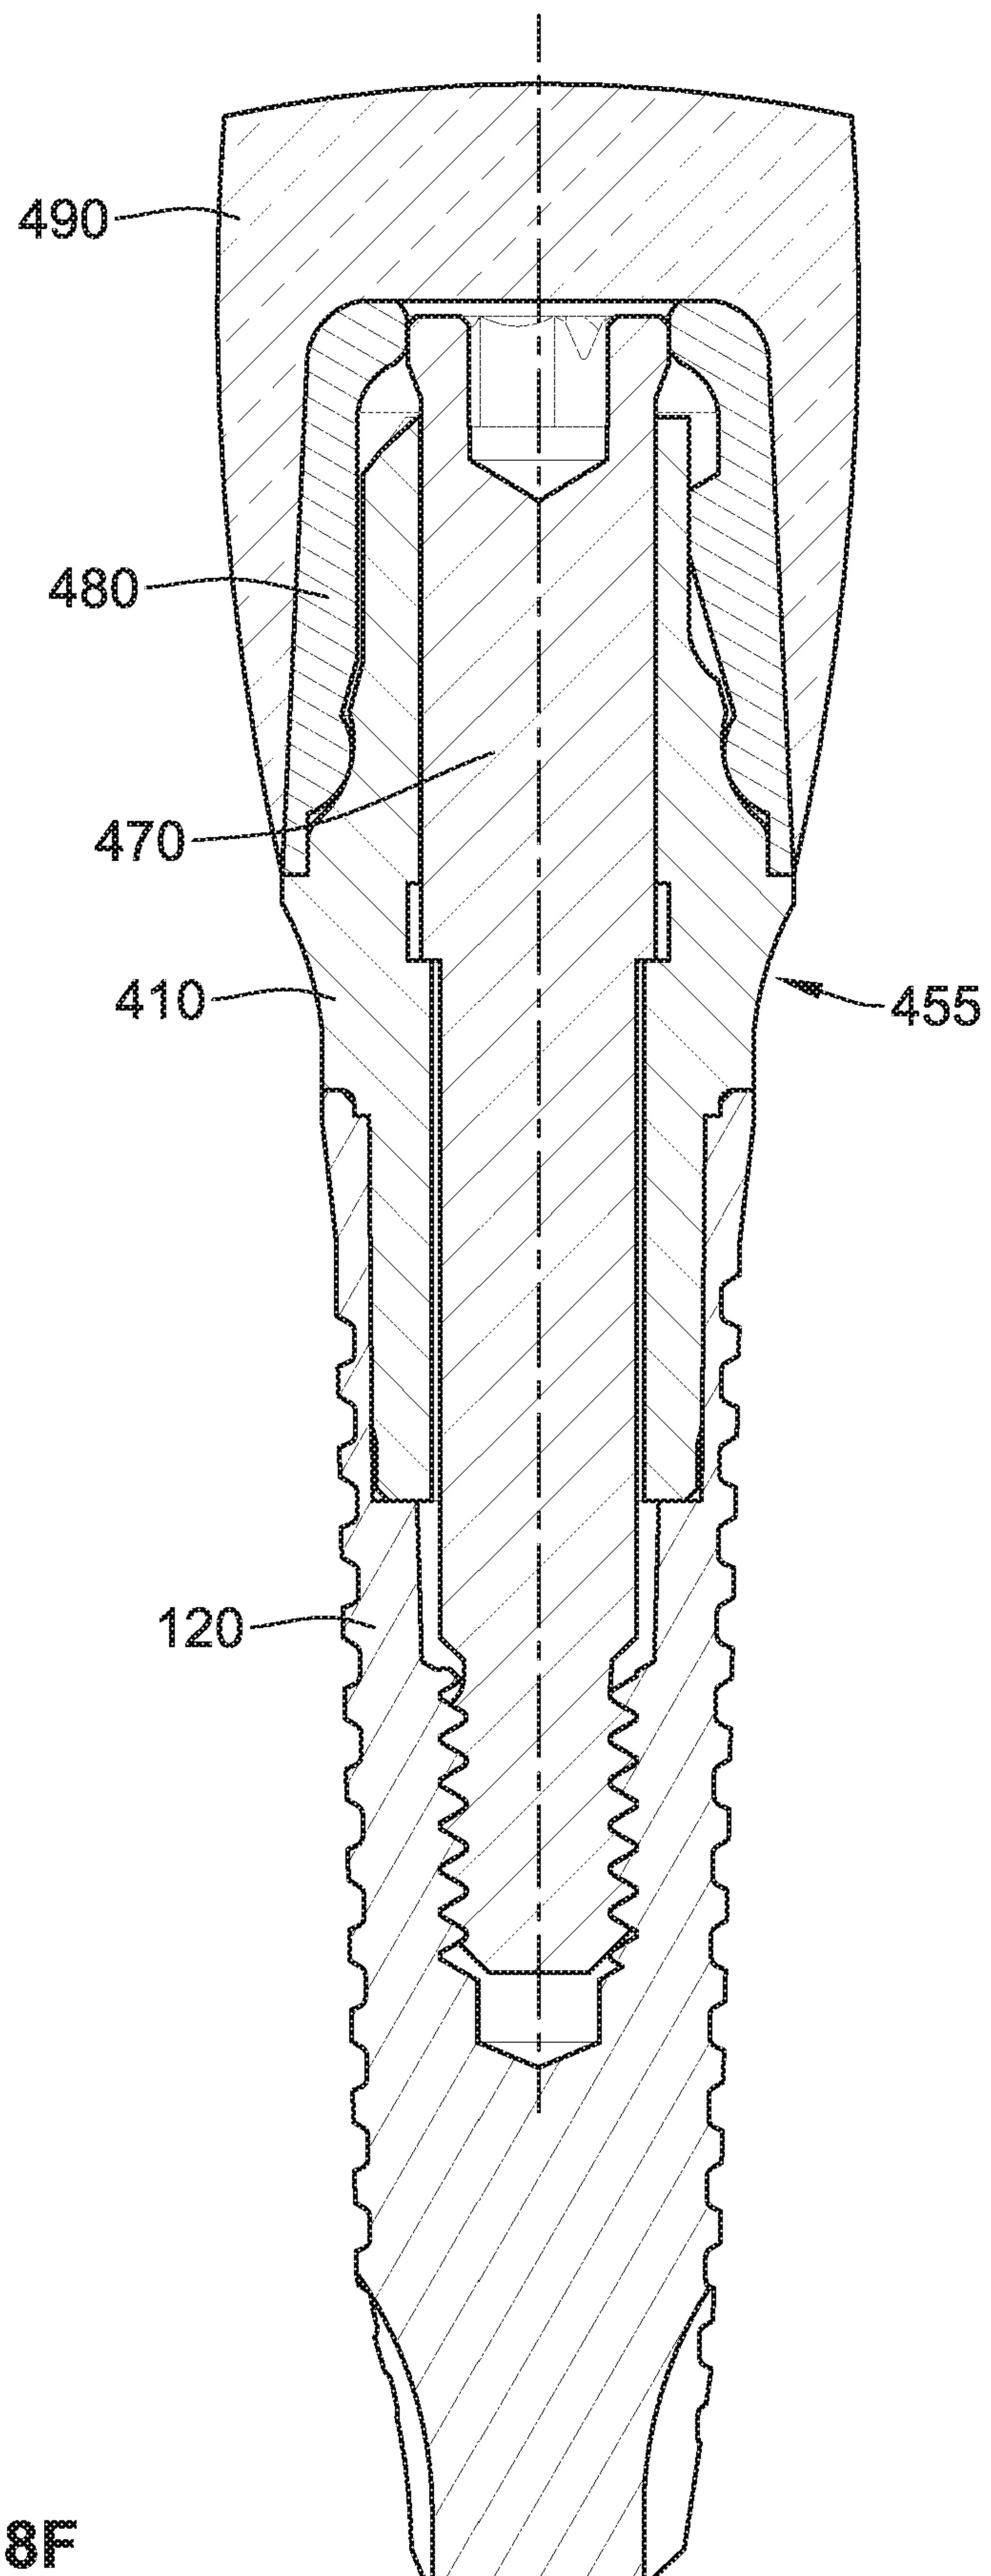


FIG. 8F



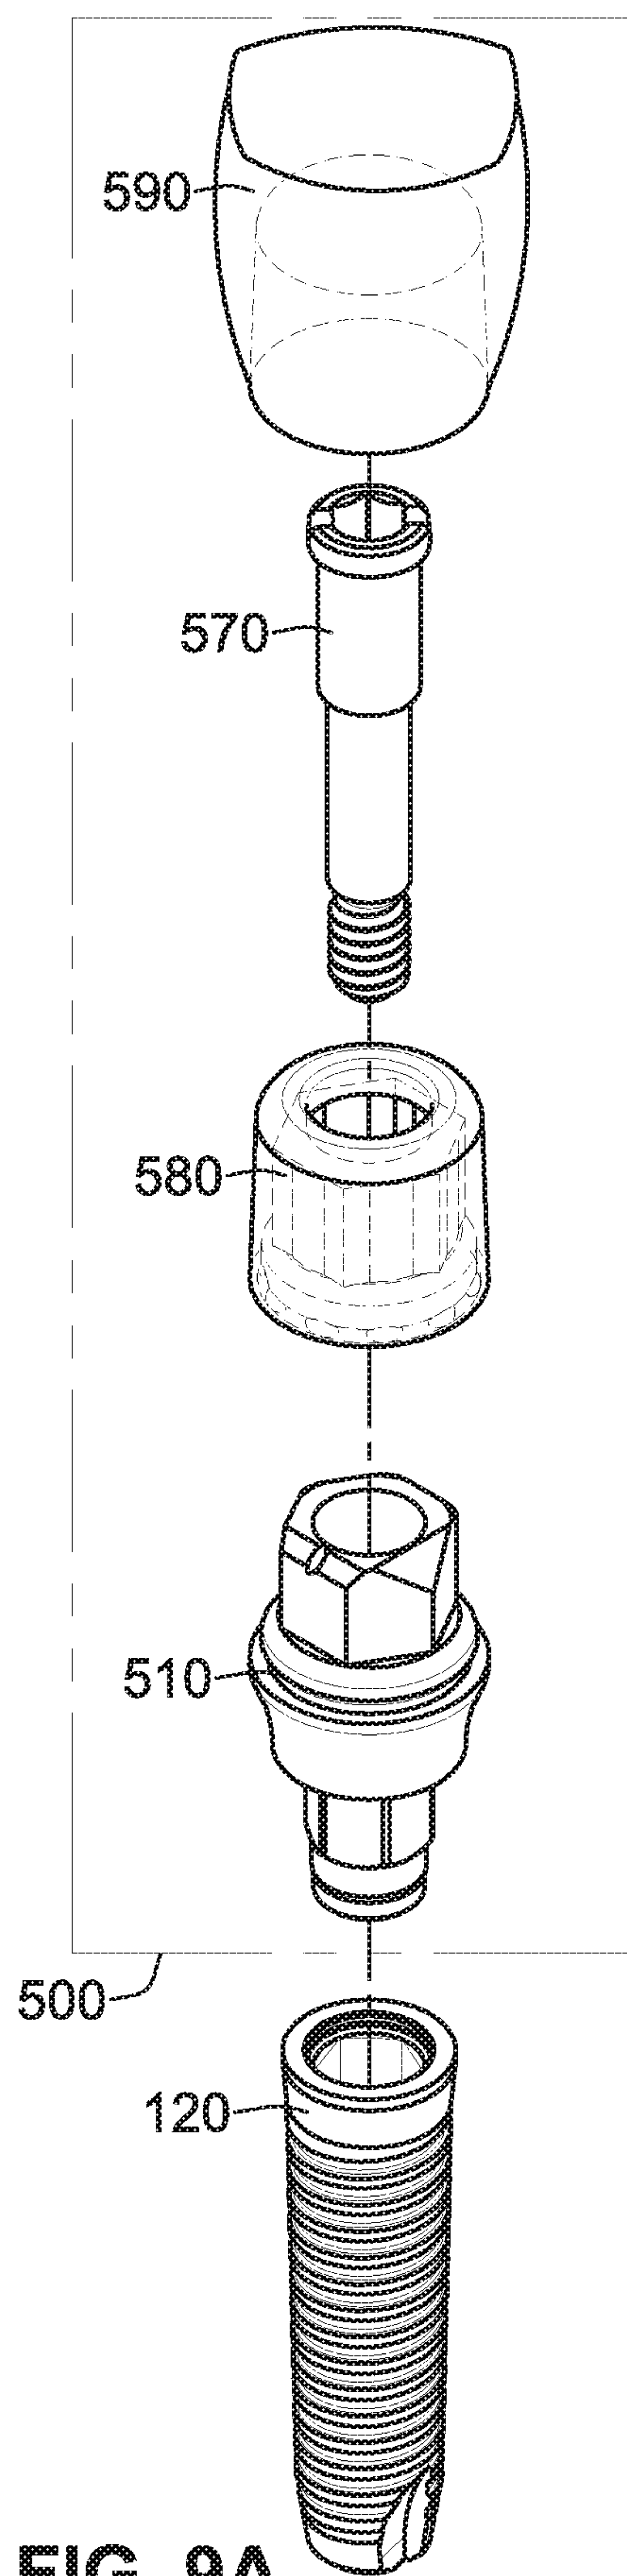


FIG. 9A

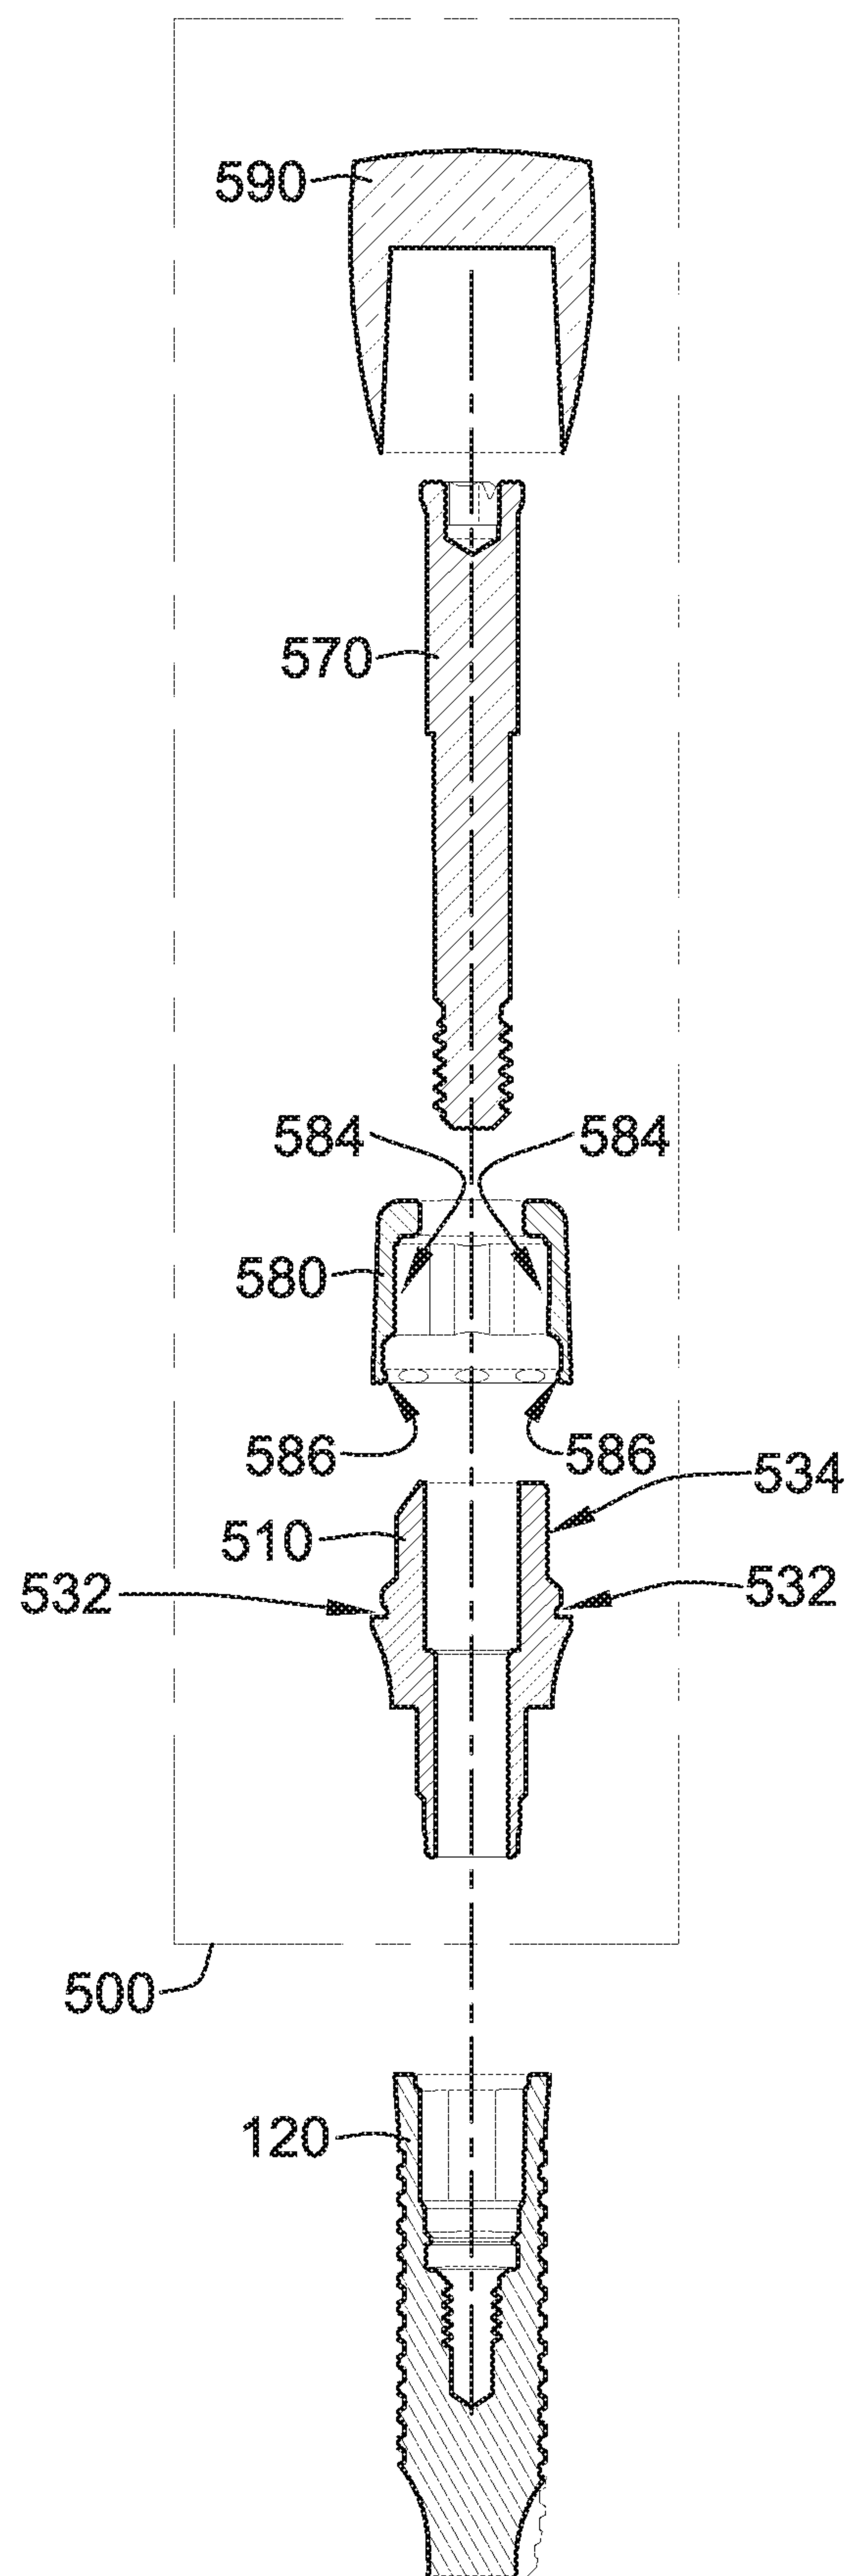
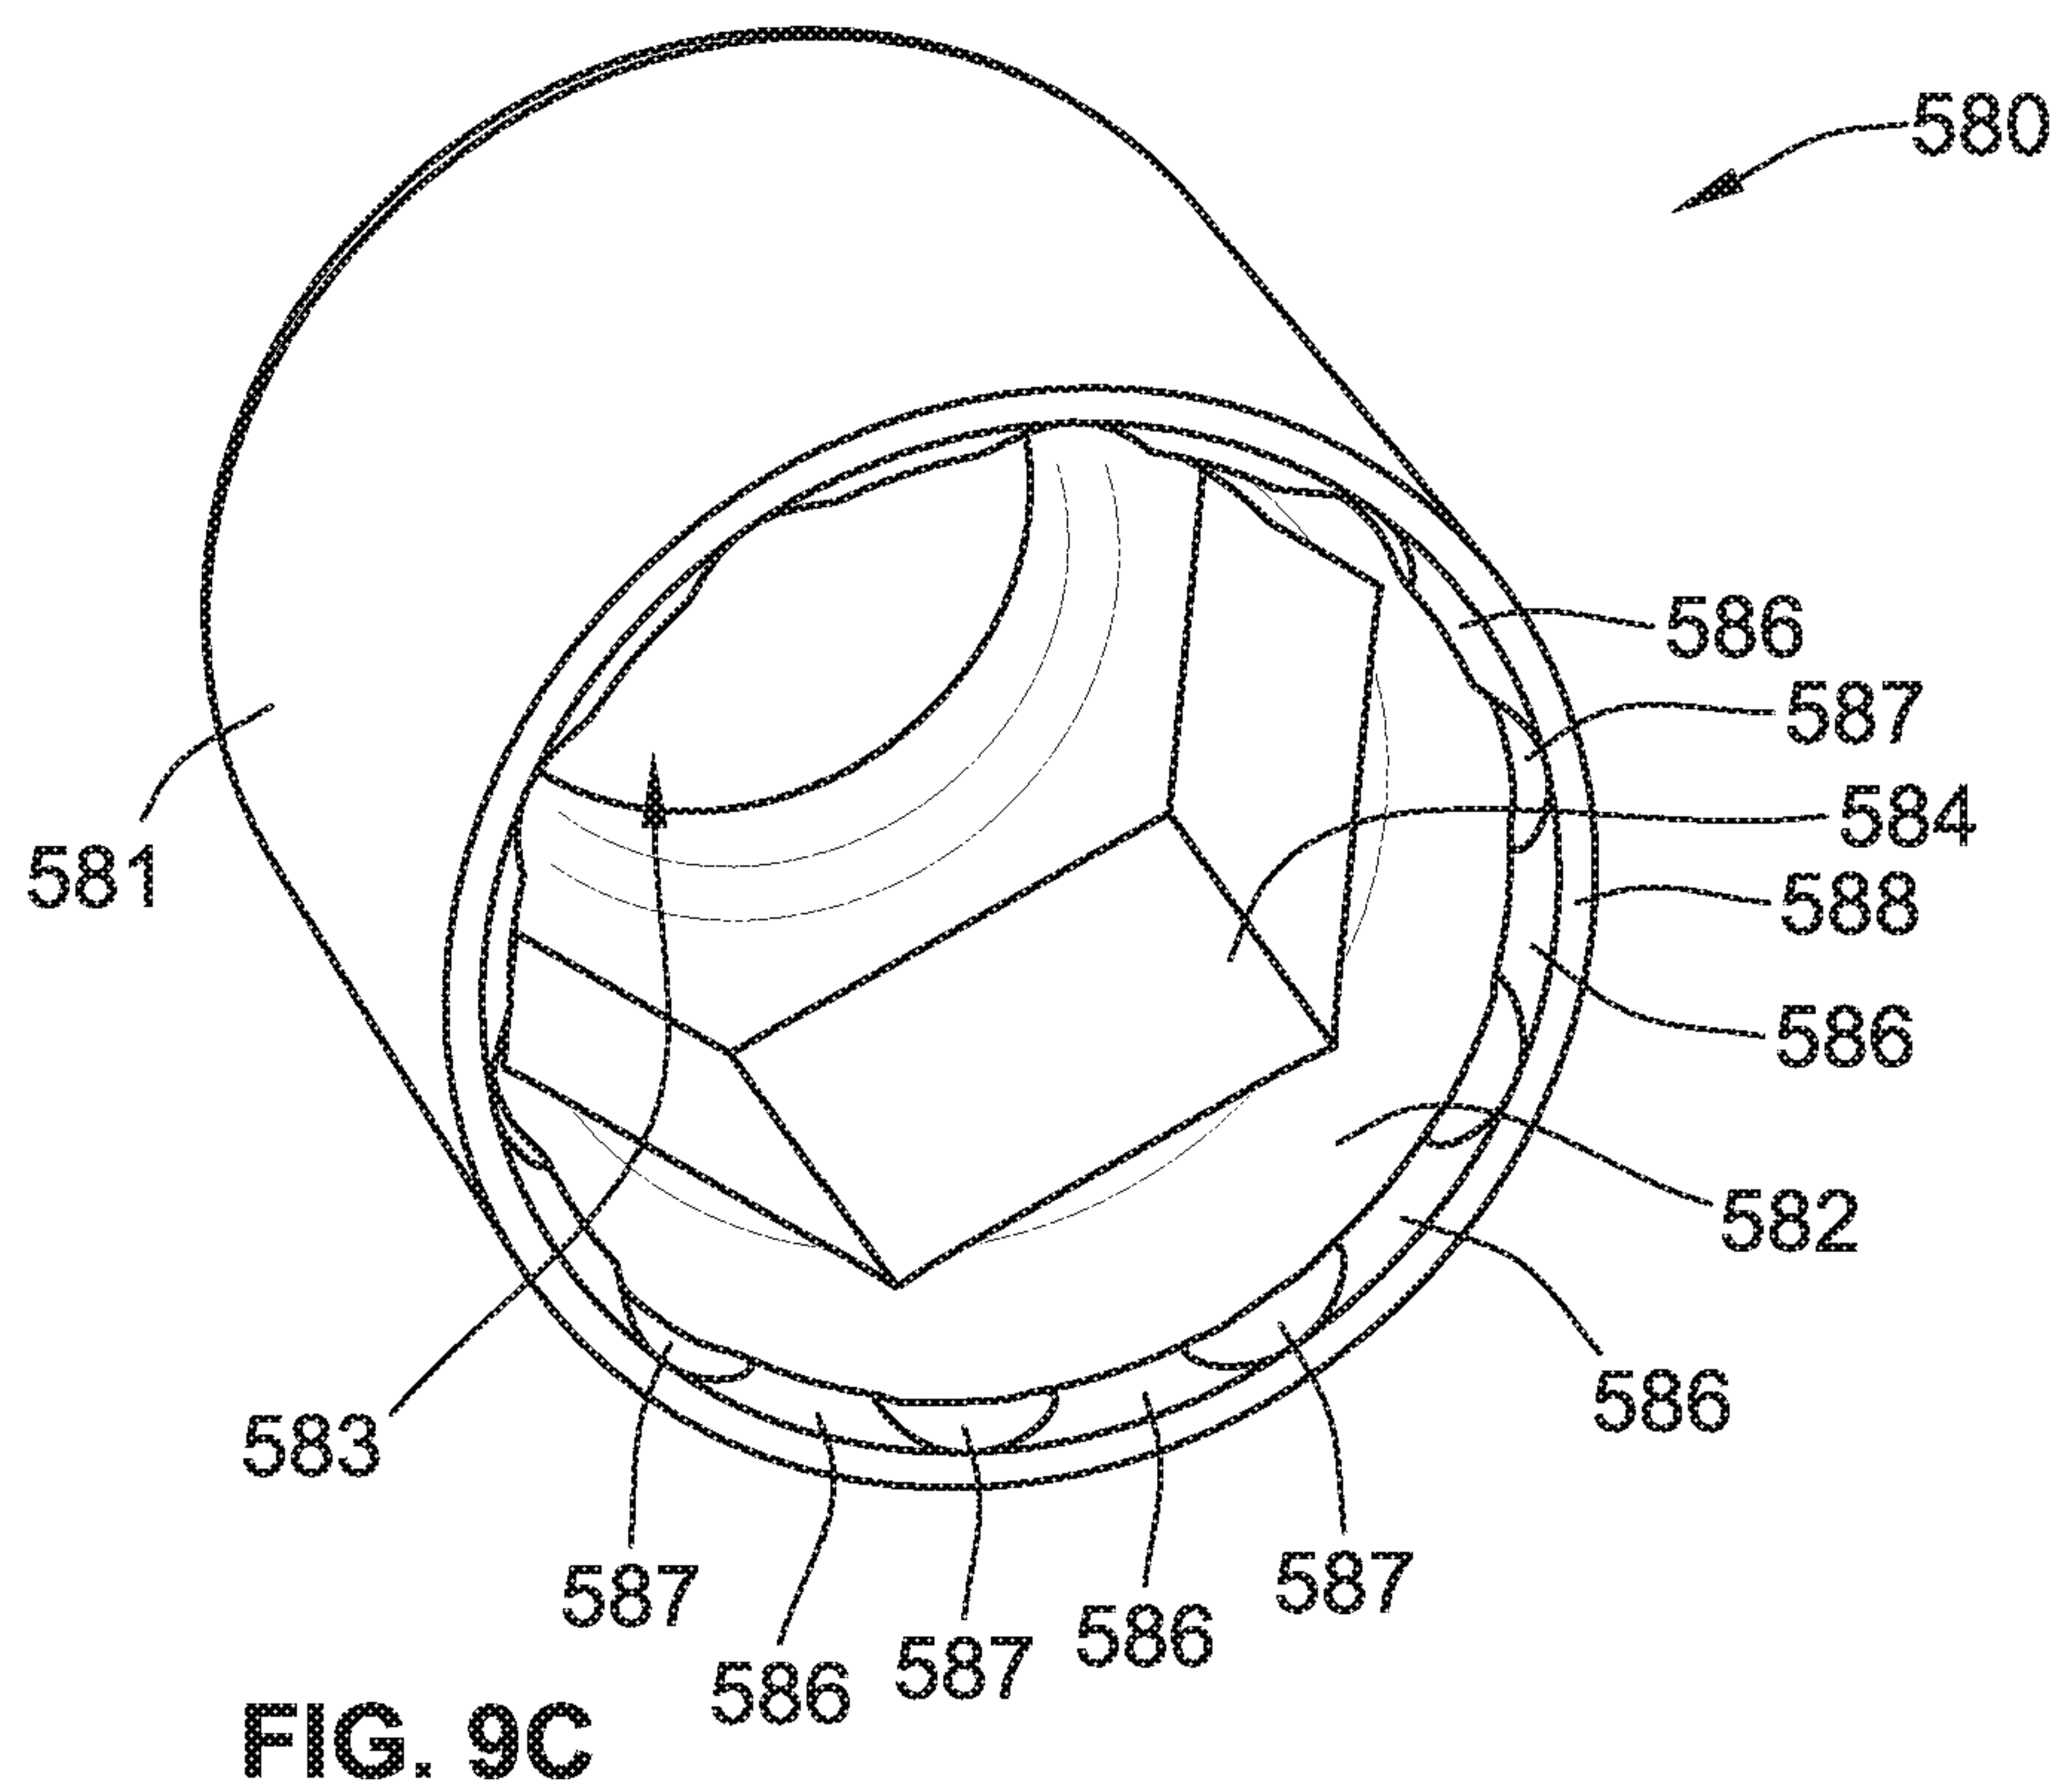
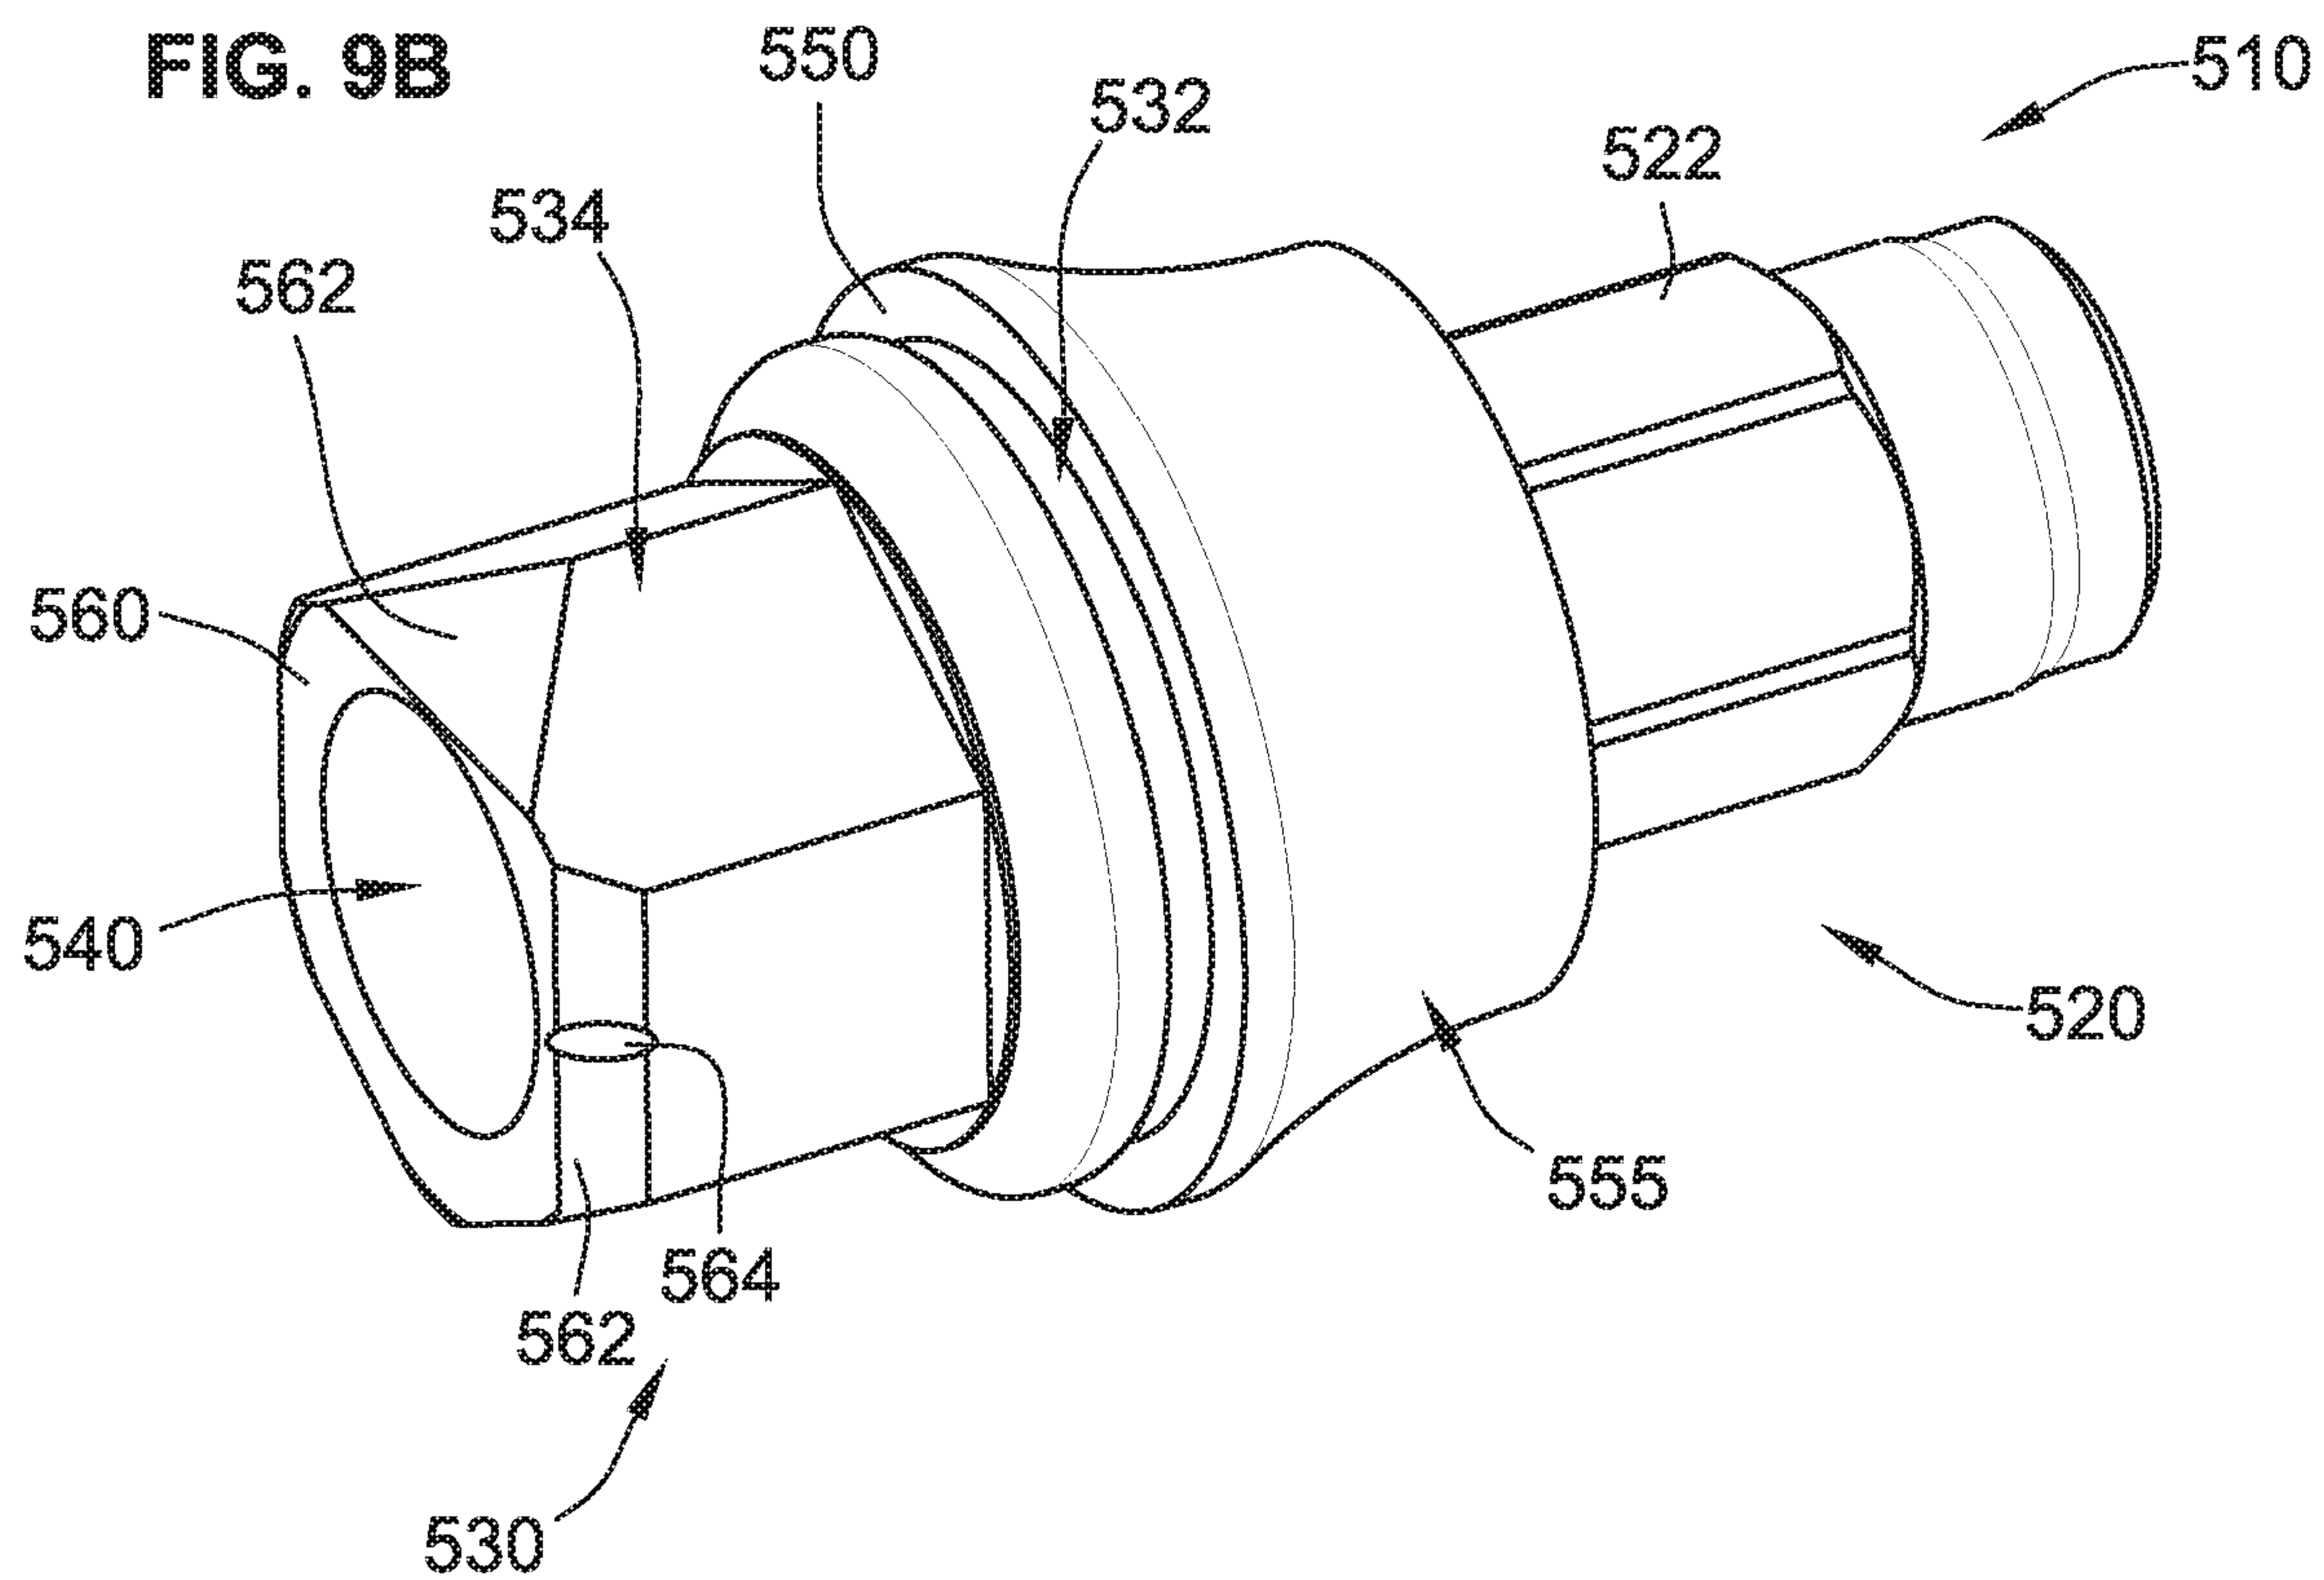


FIG. 9D





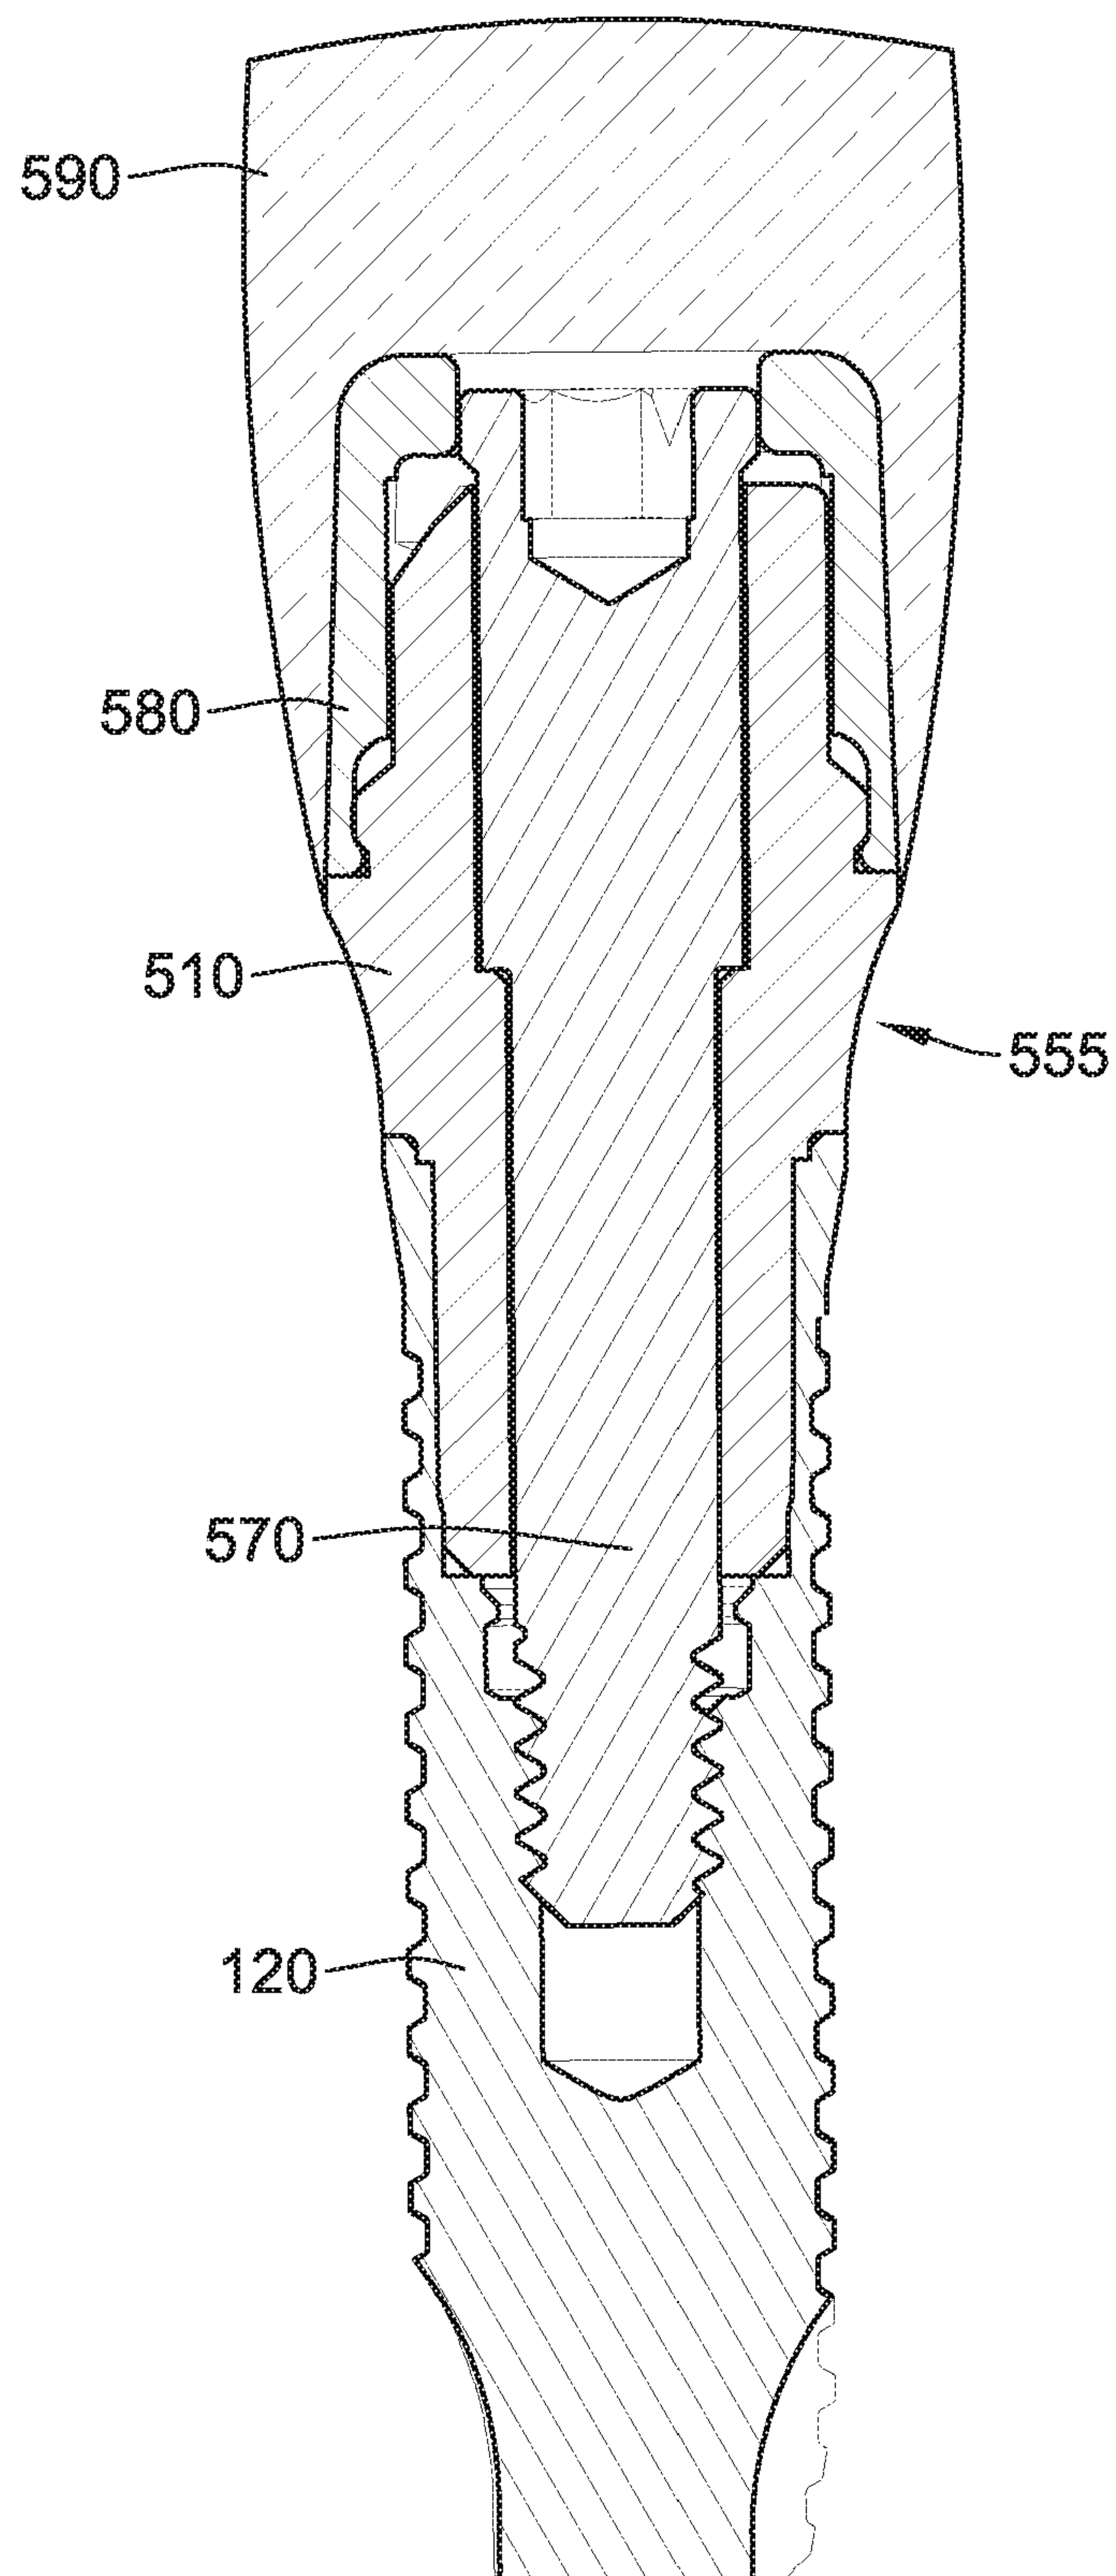


FIG. 9E

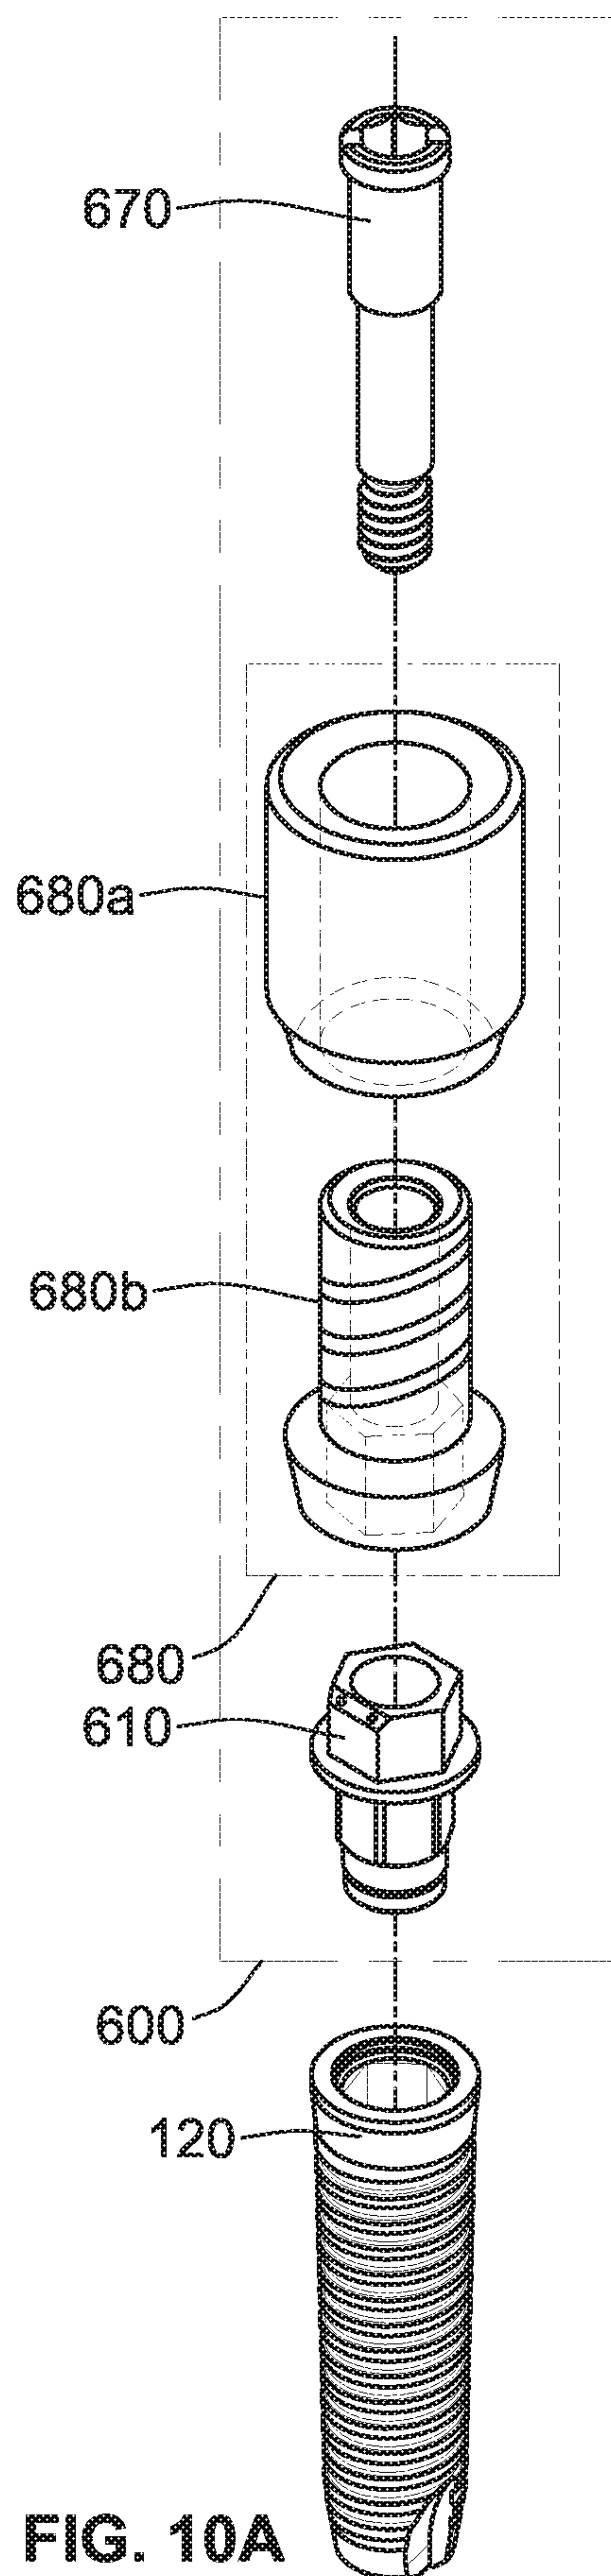


FIG. 10A

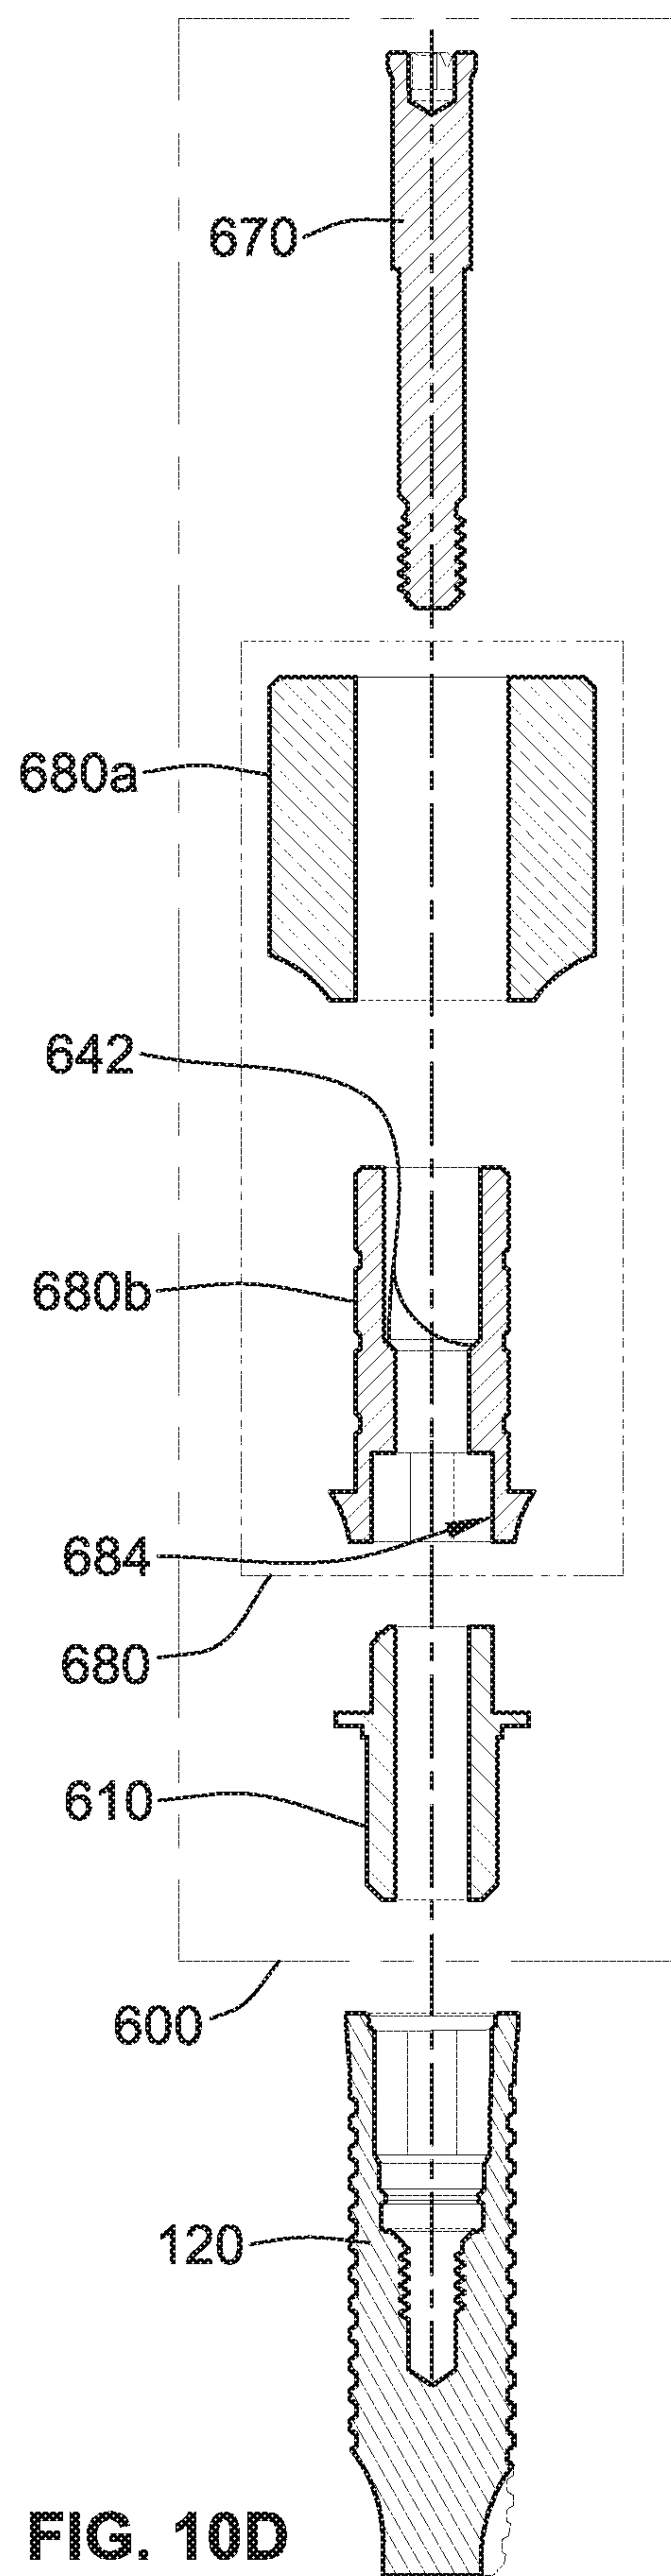
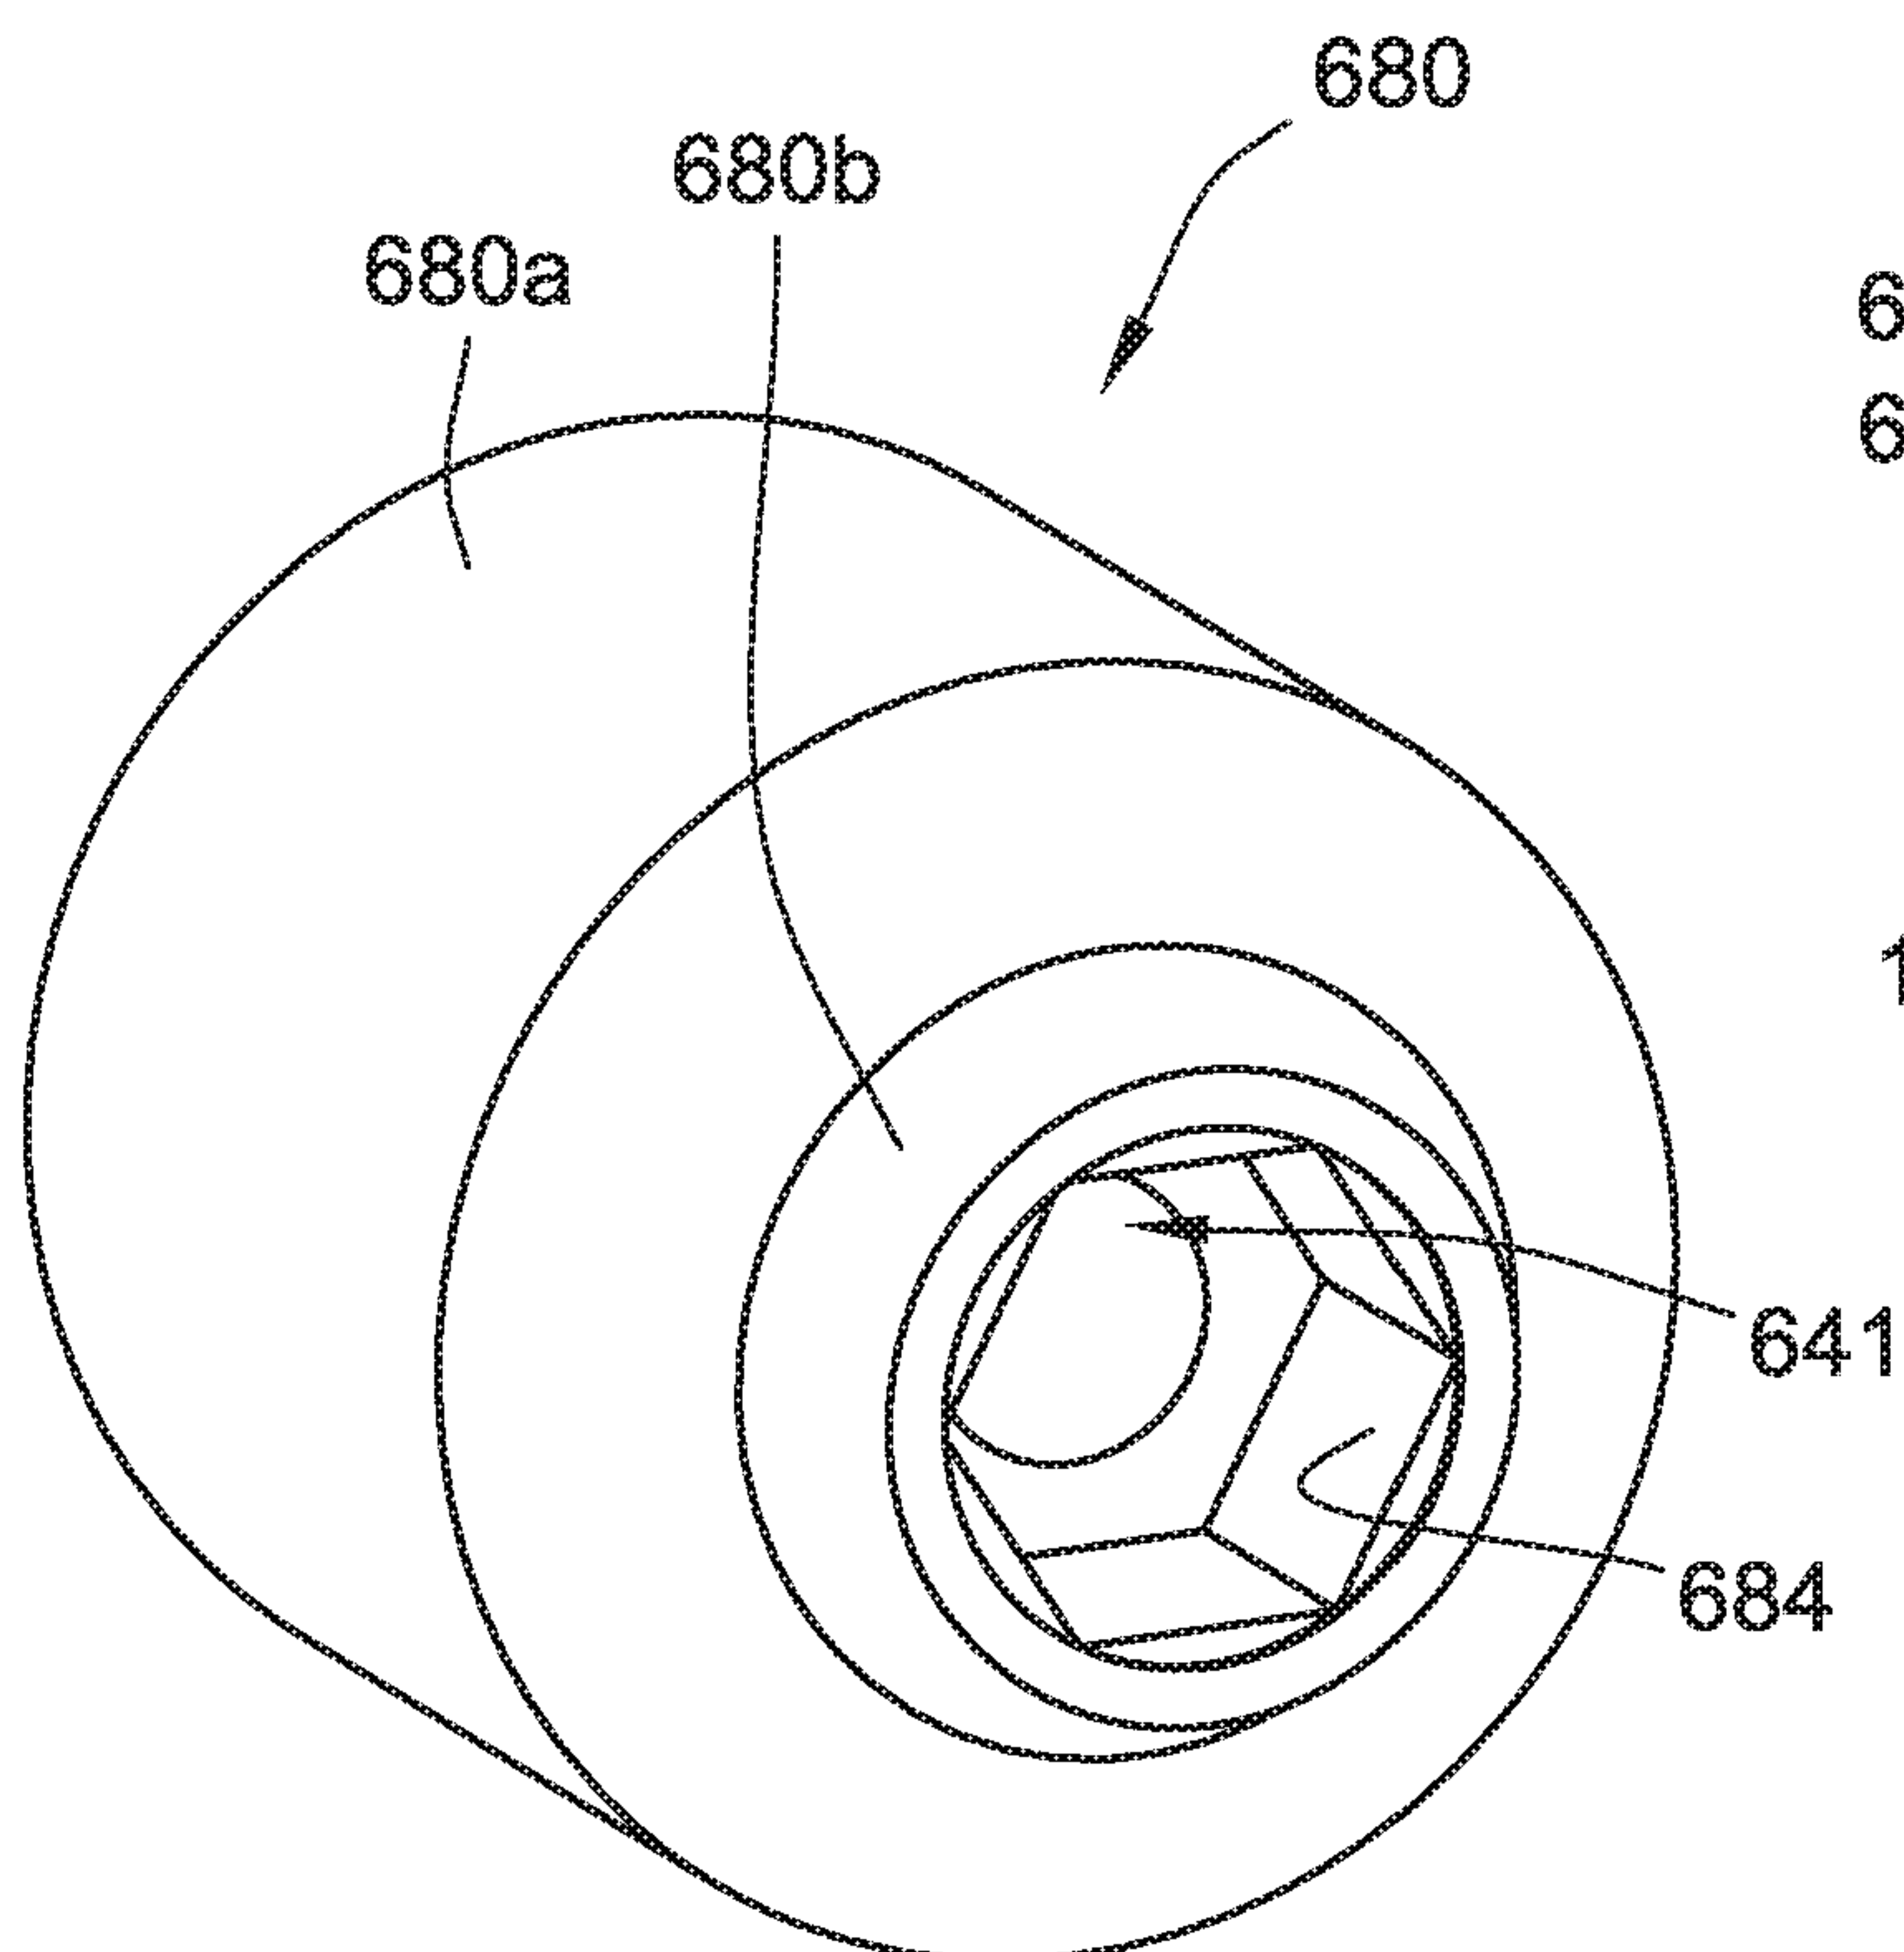
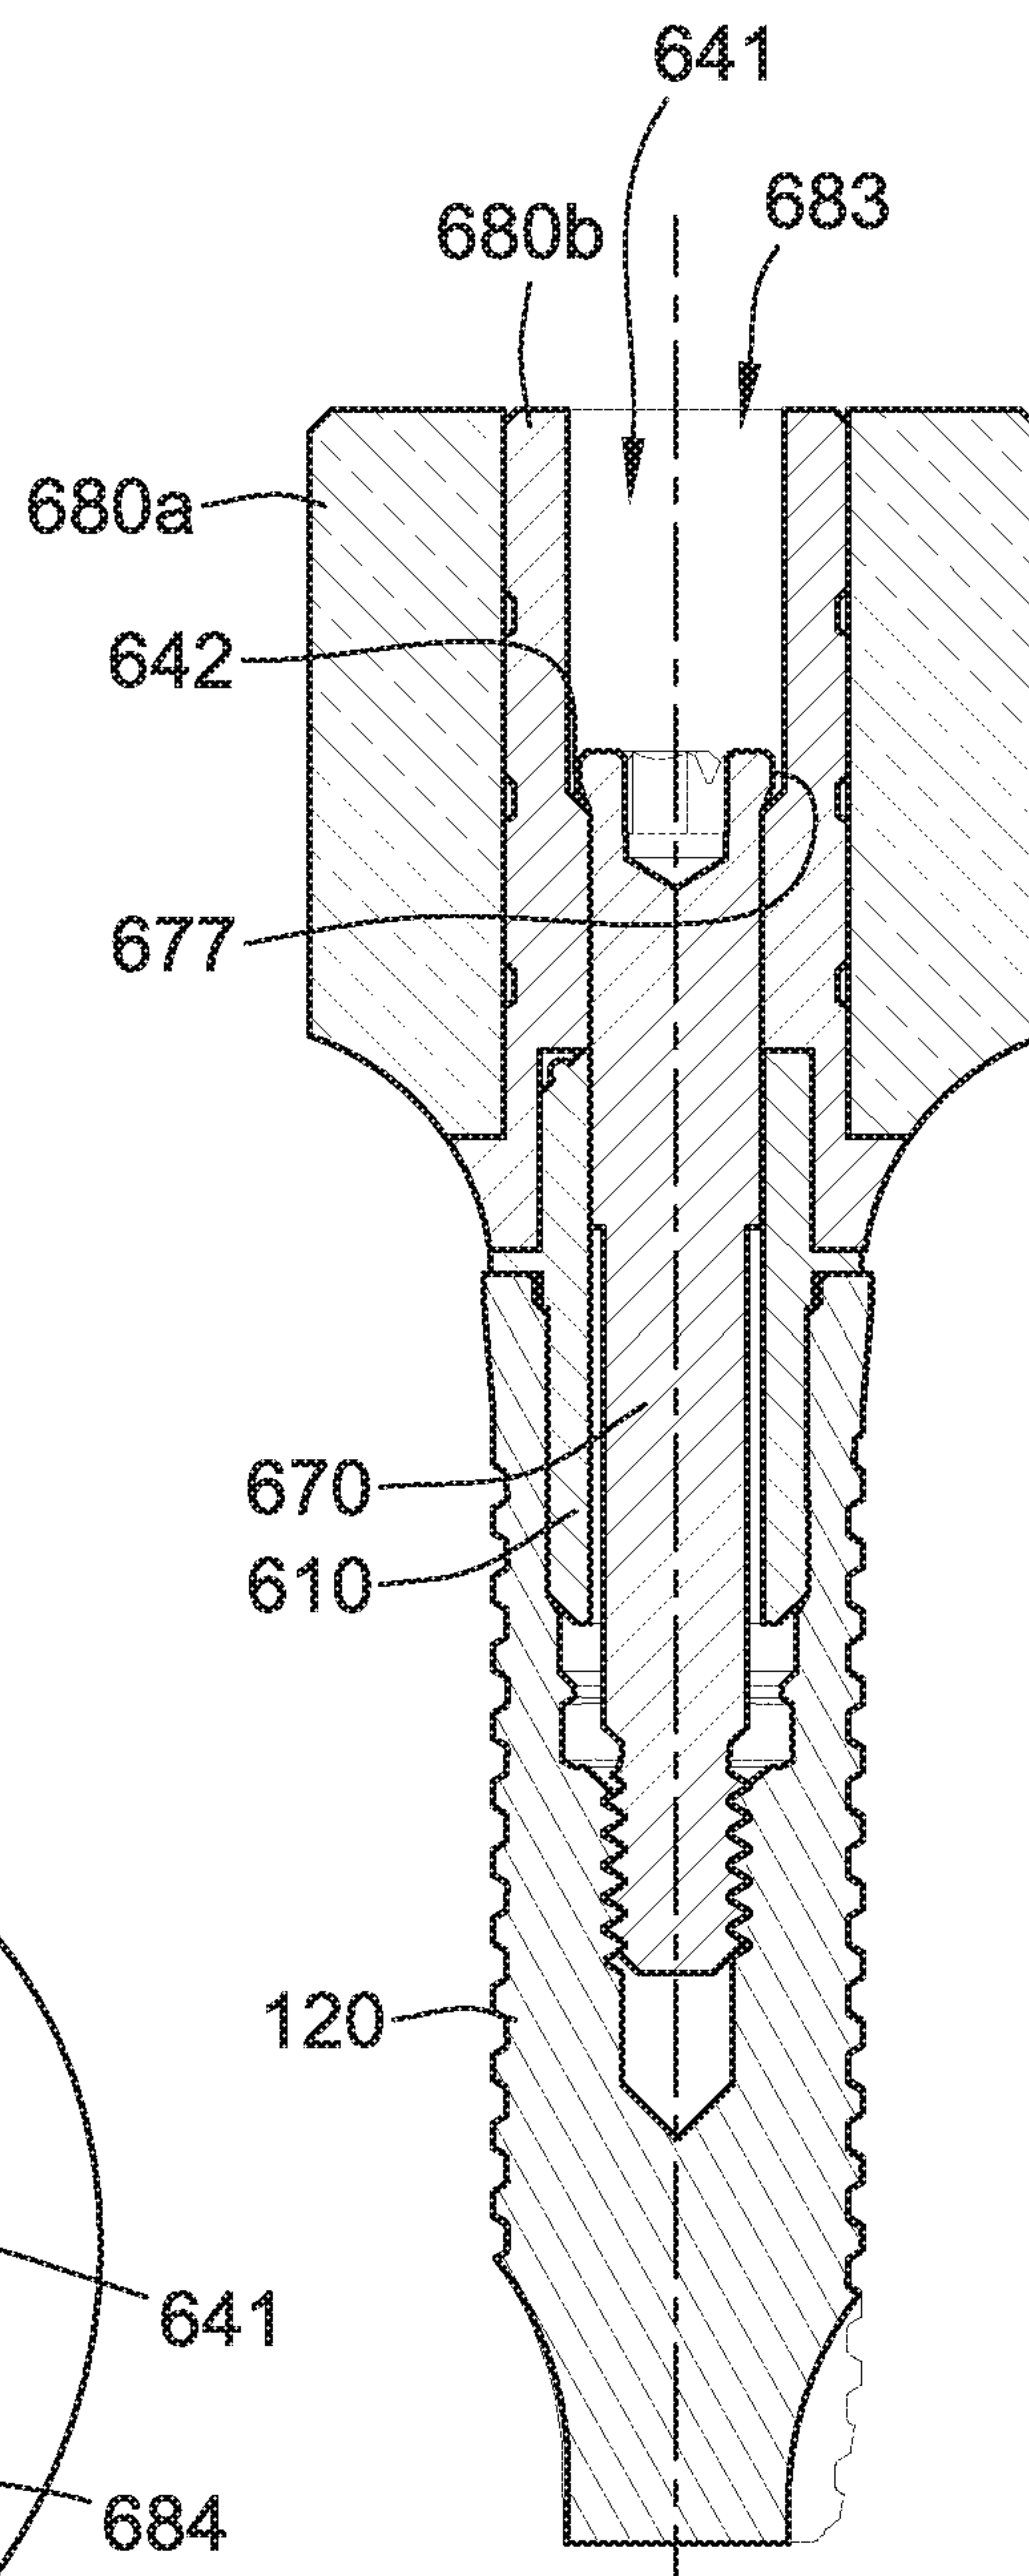
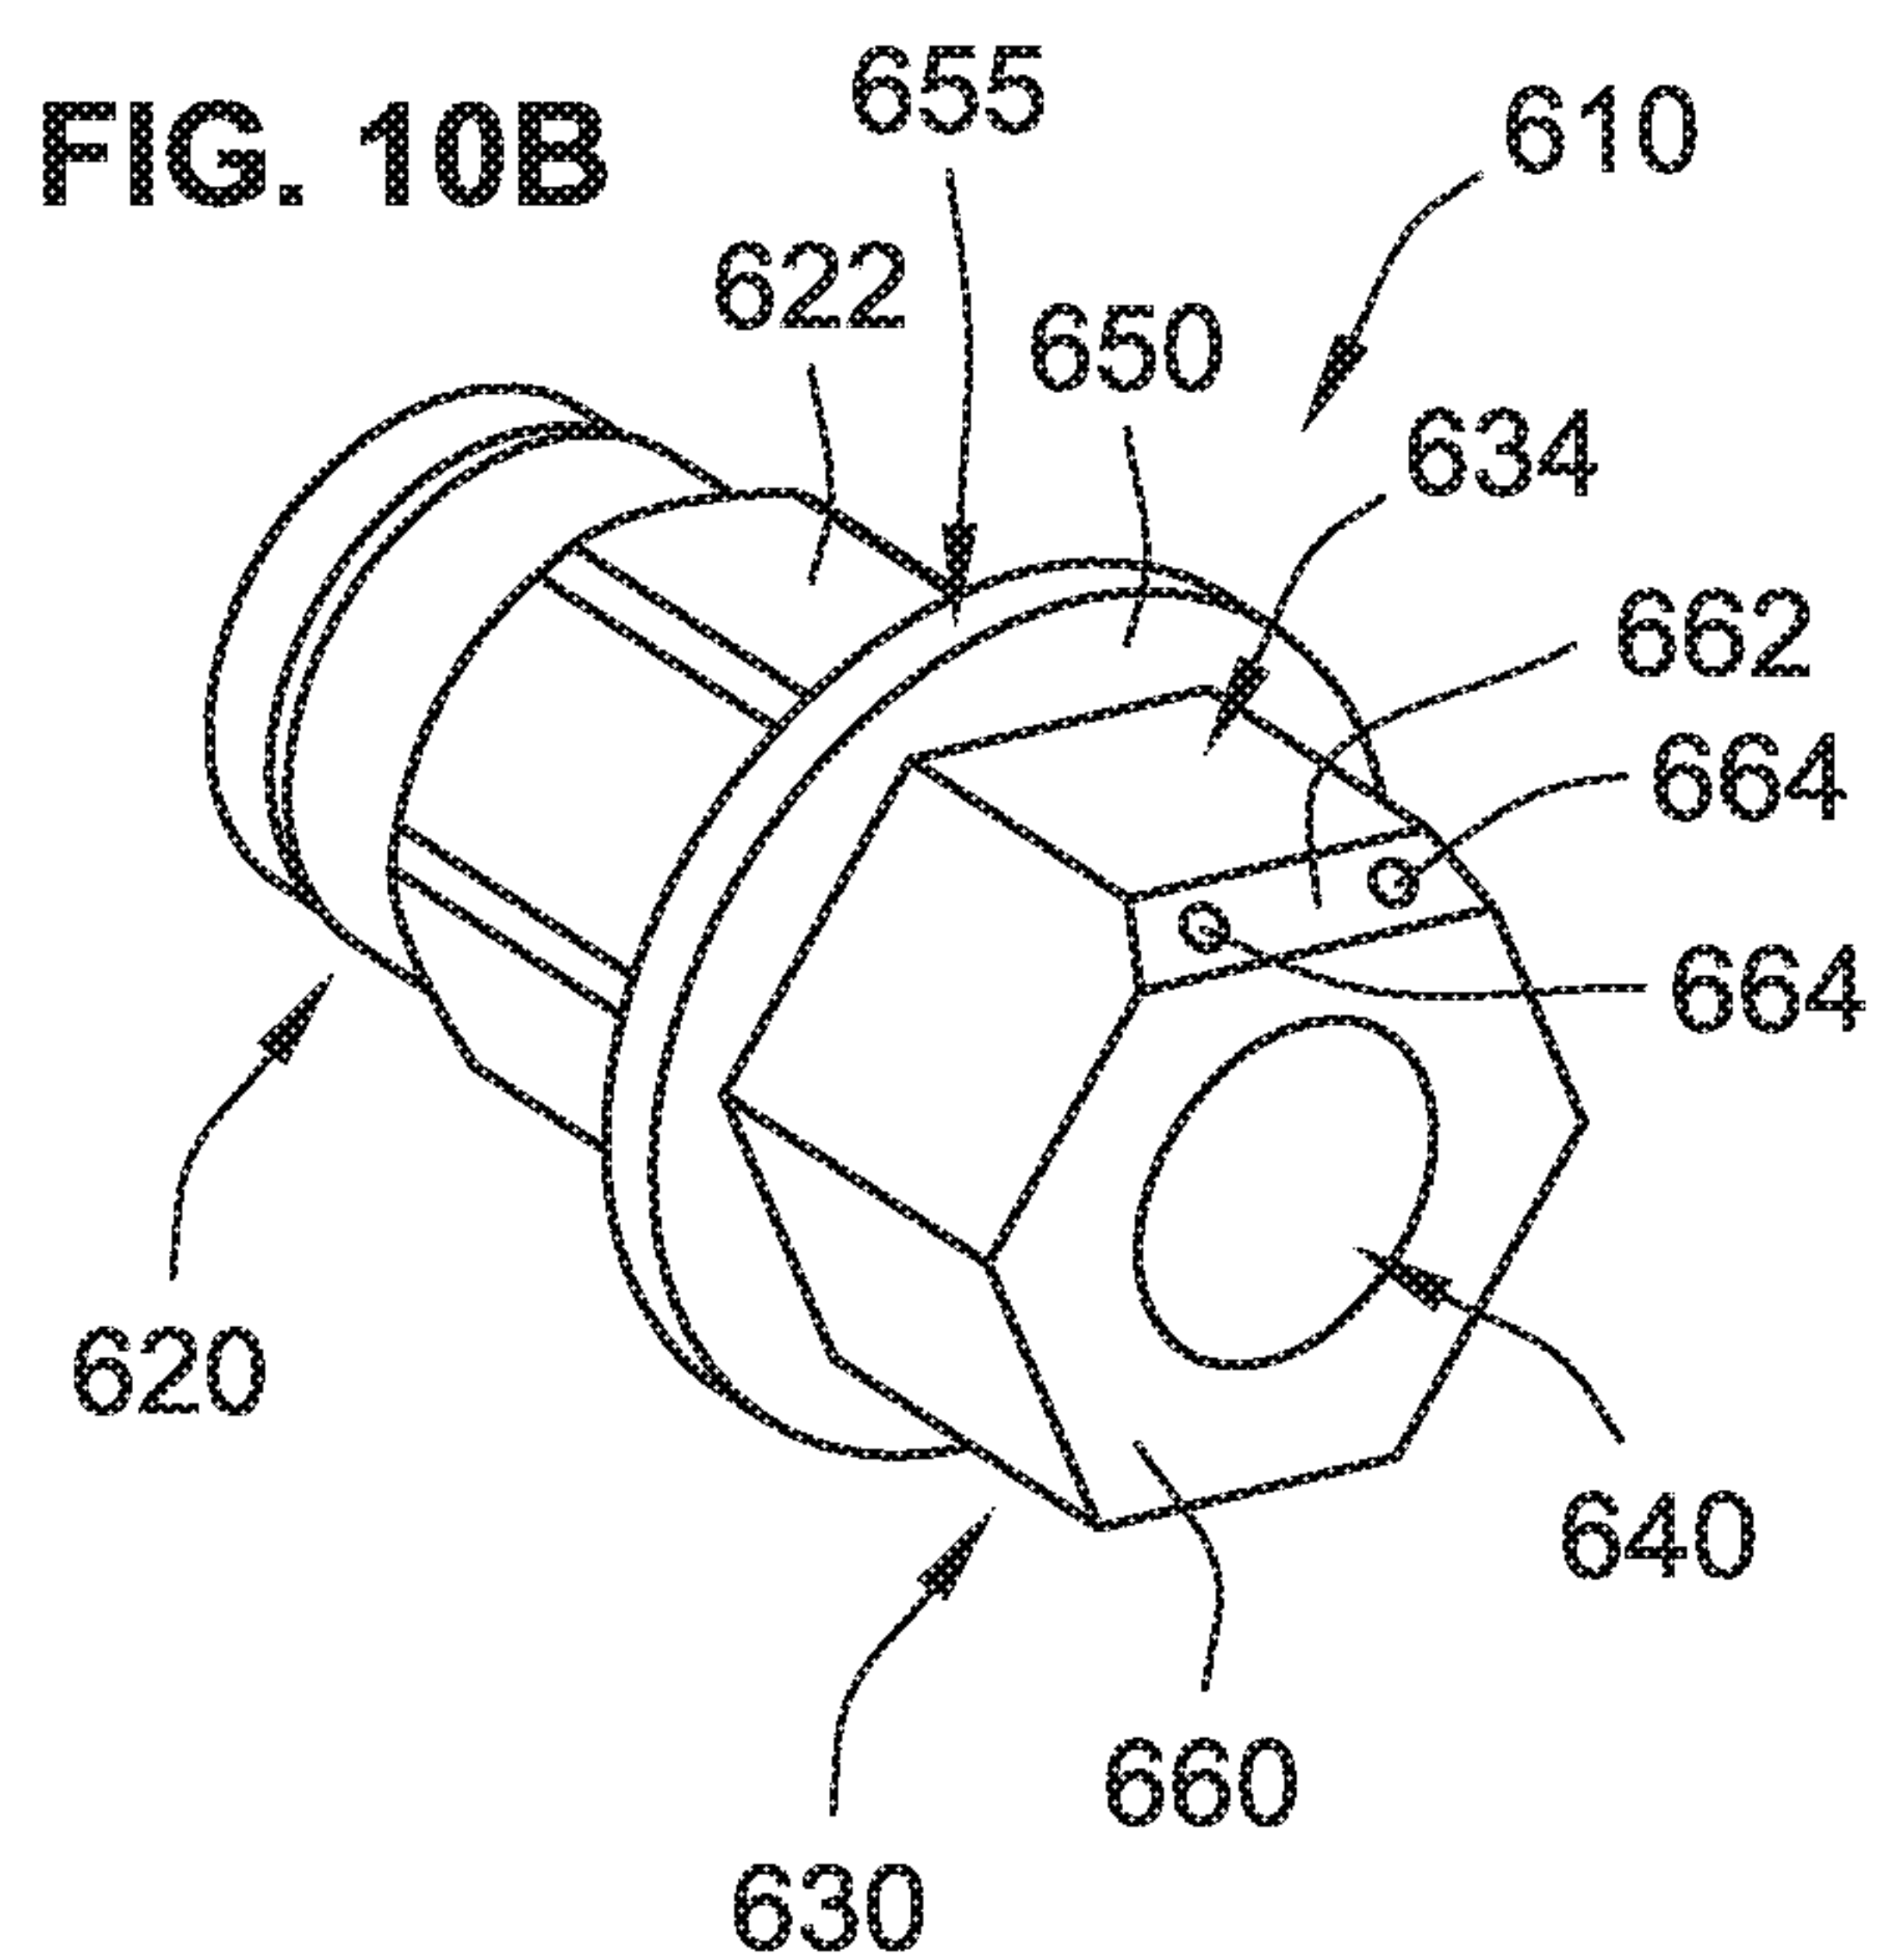


FIG. 10D





**FIG. 10E**

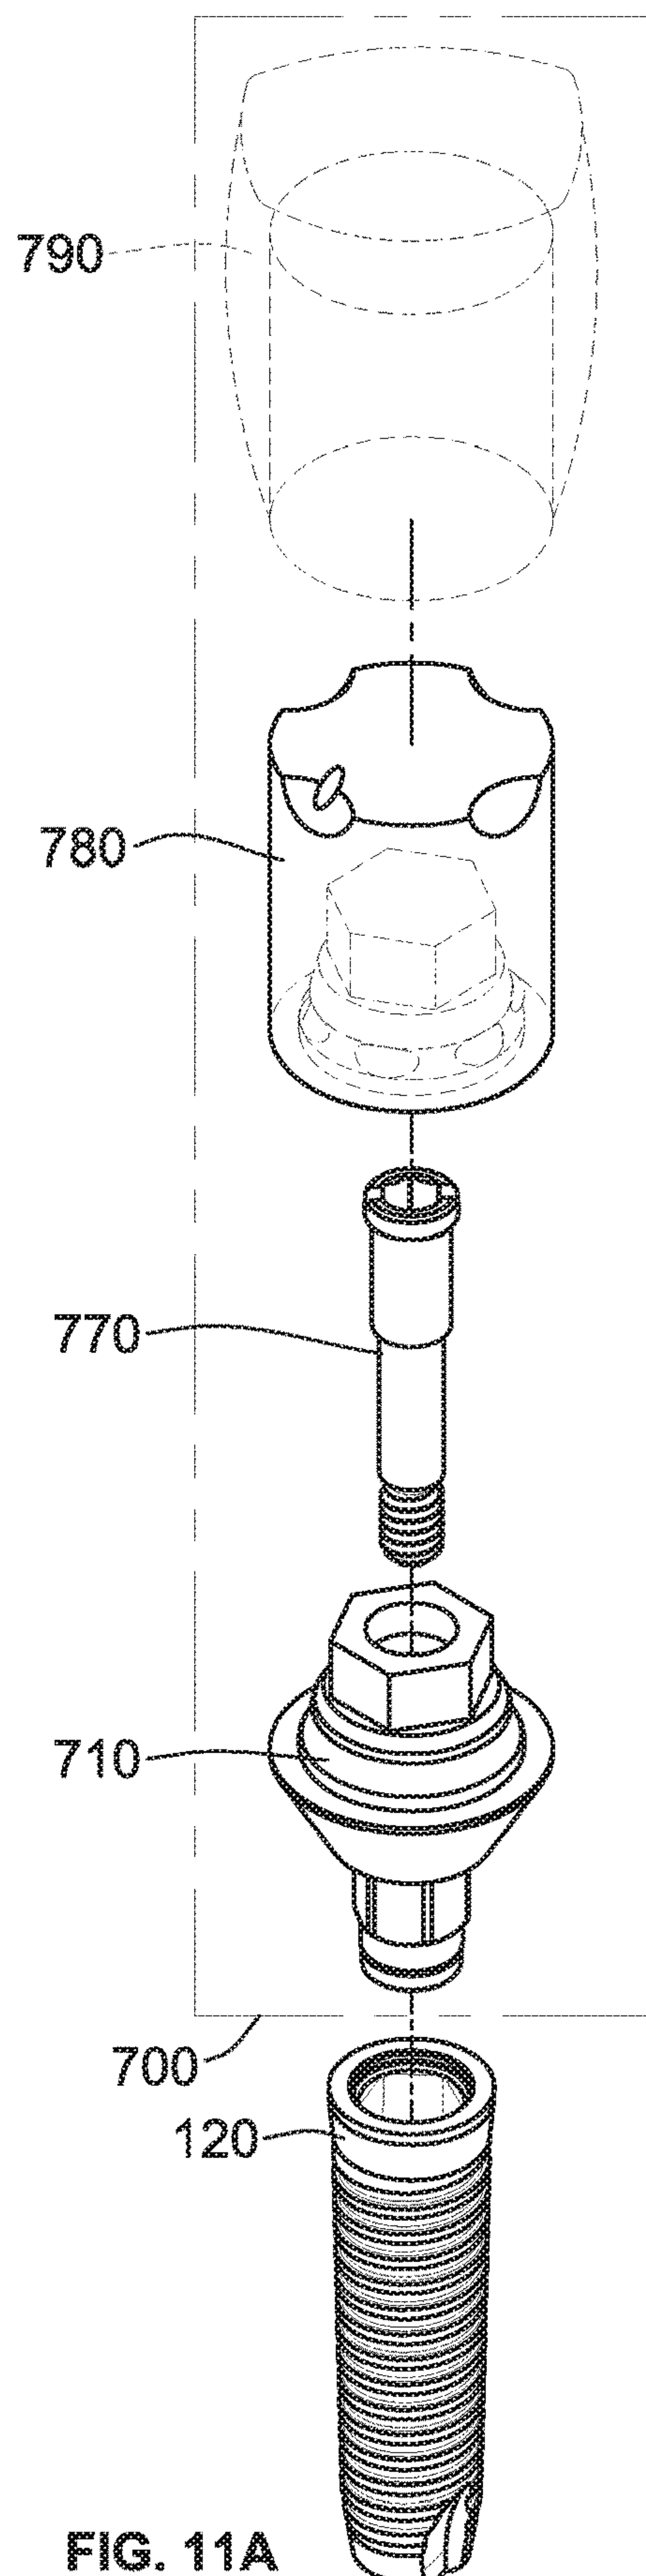


FIG. 11A

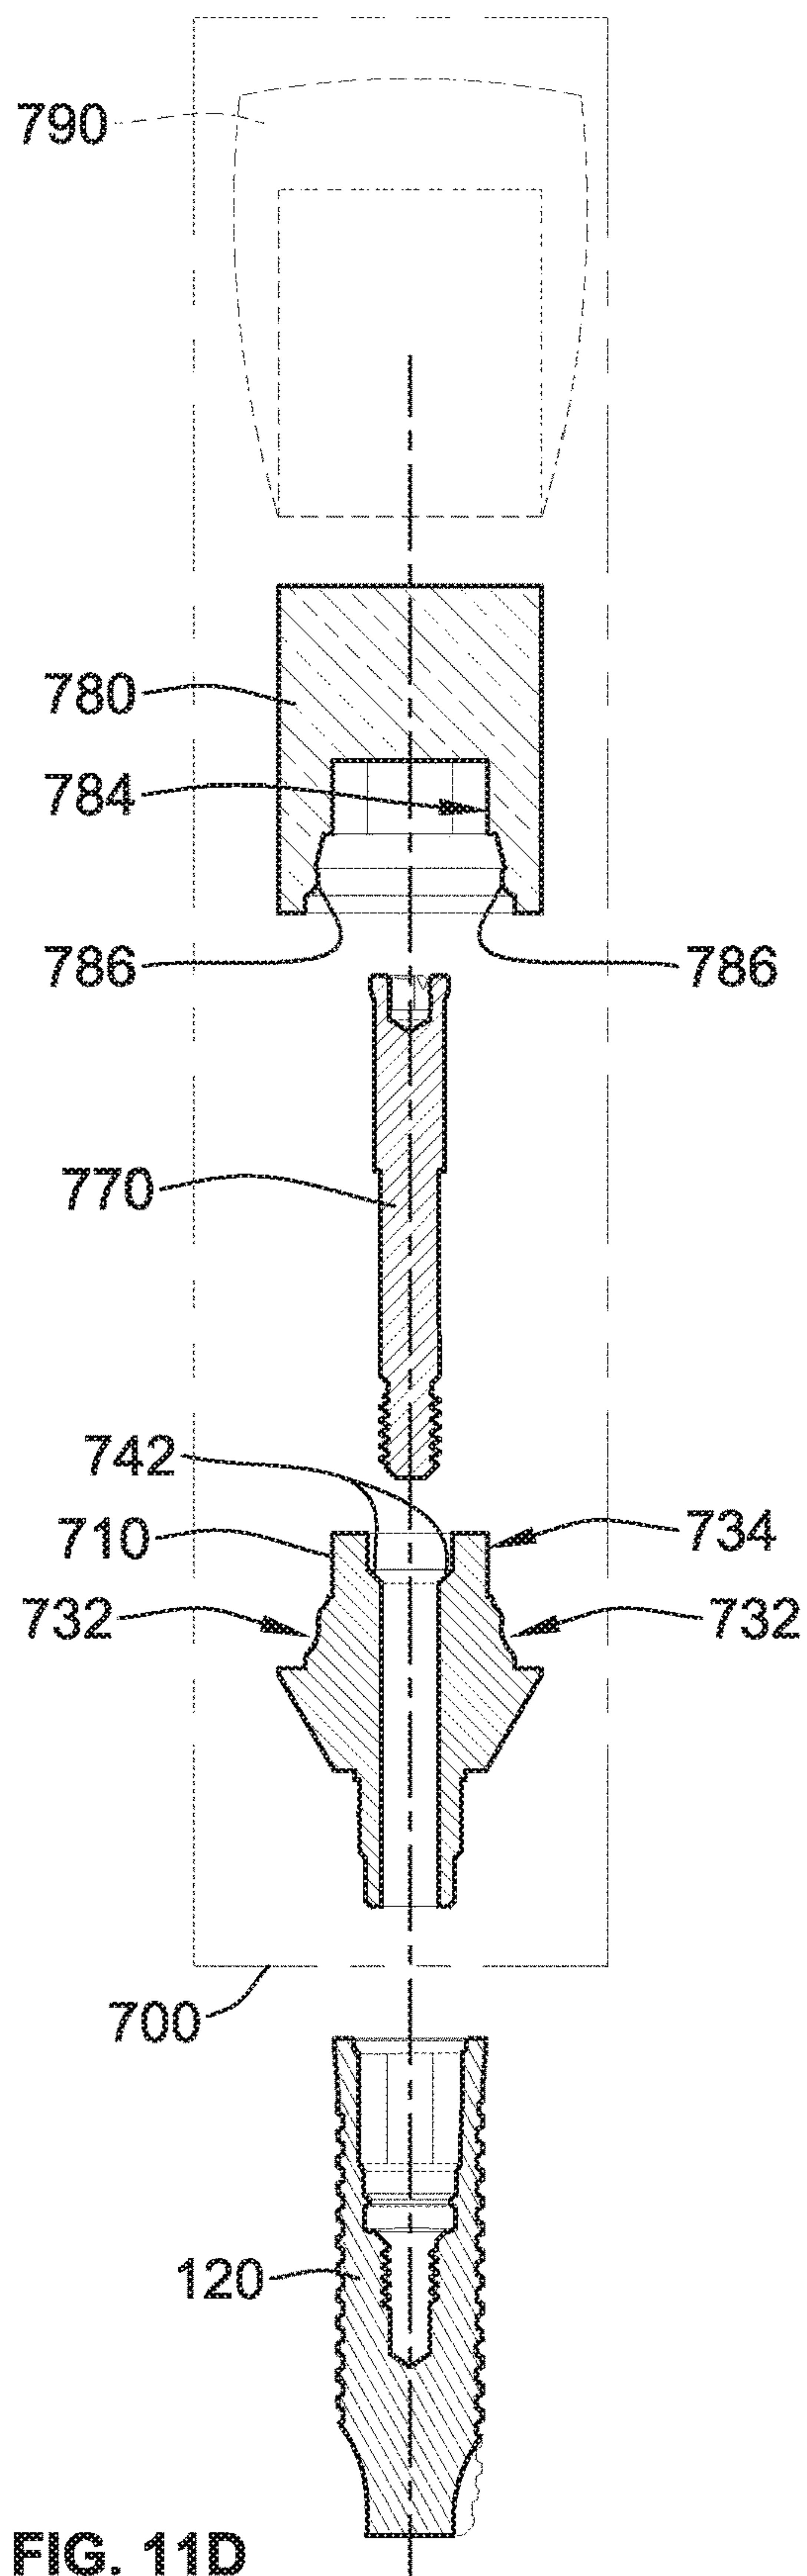


FIG. 11D



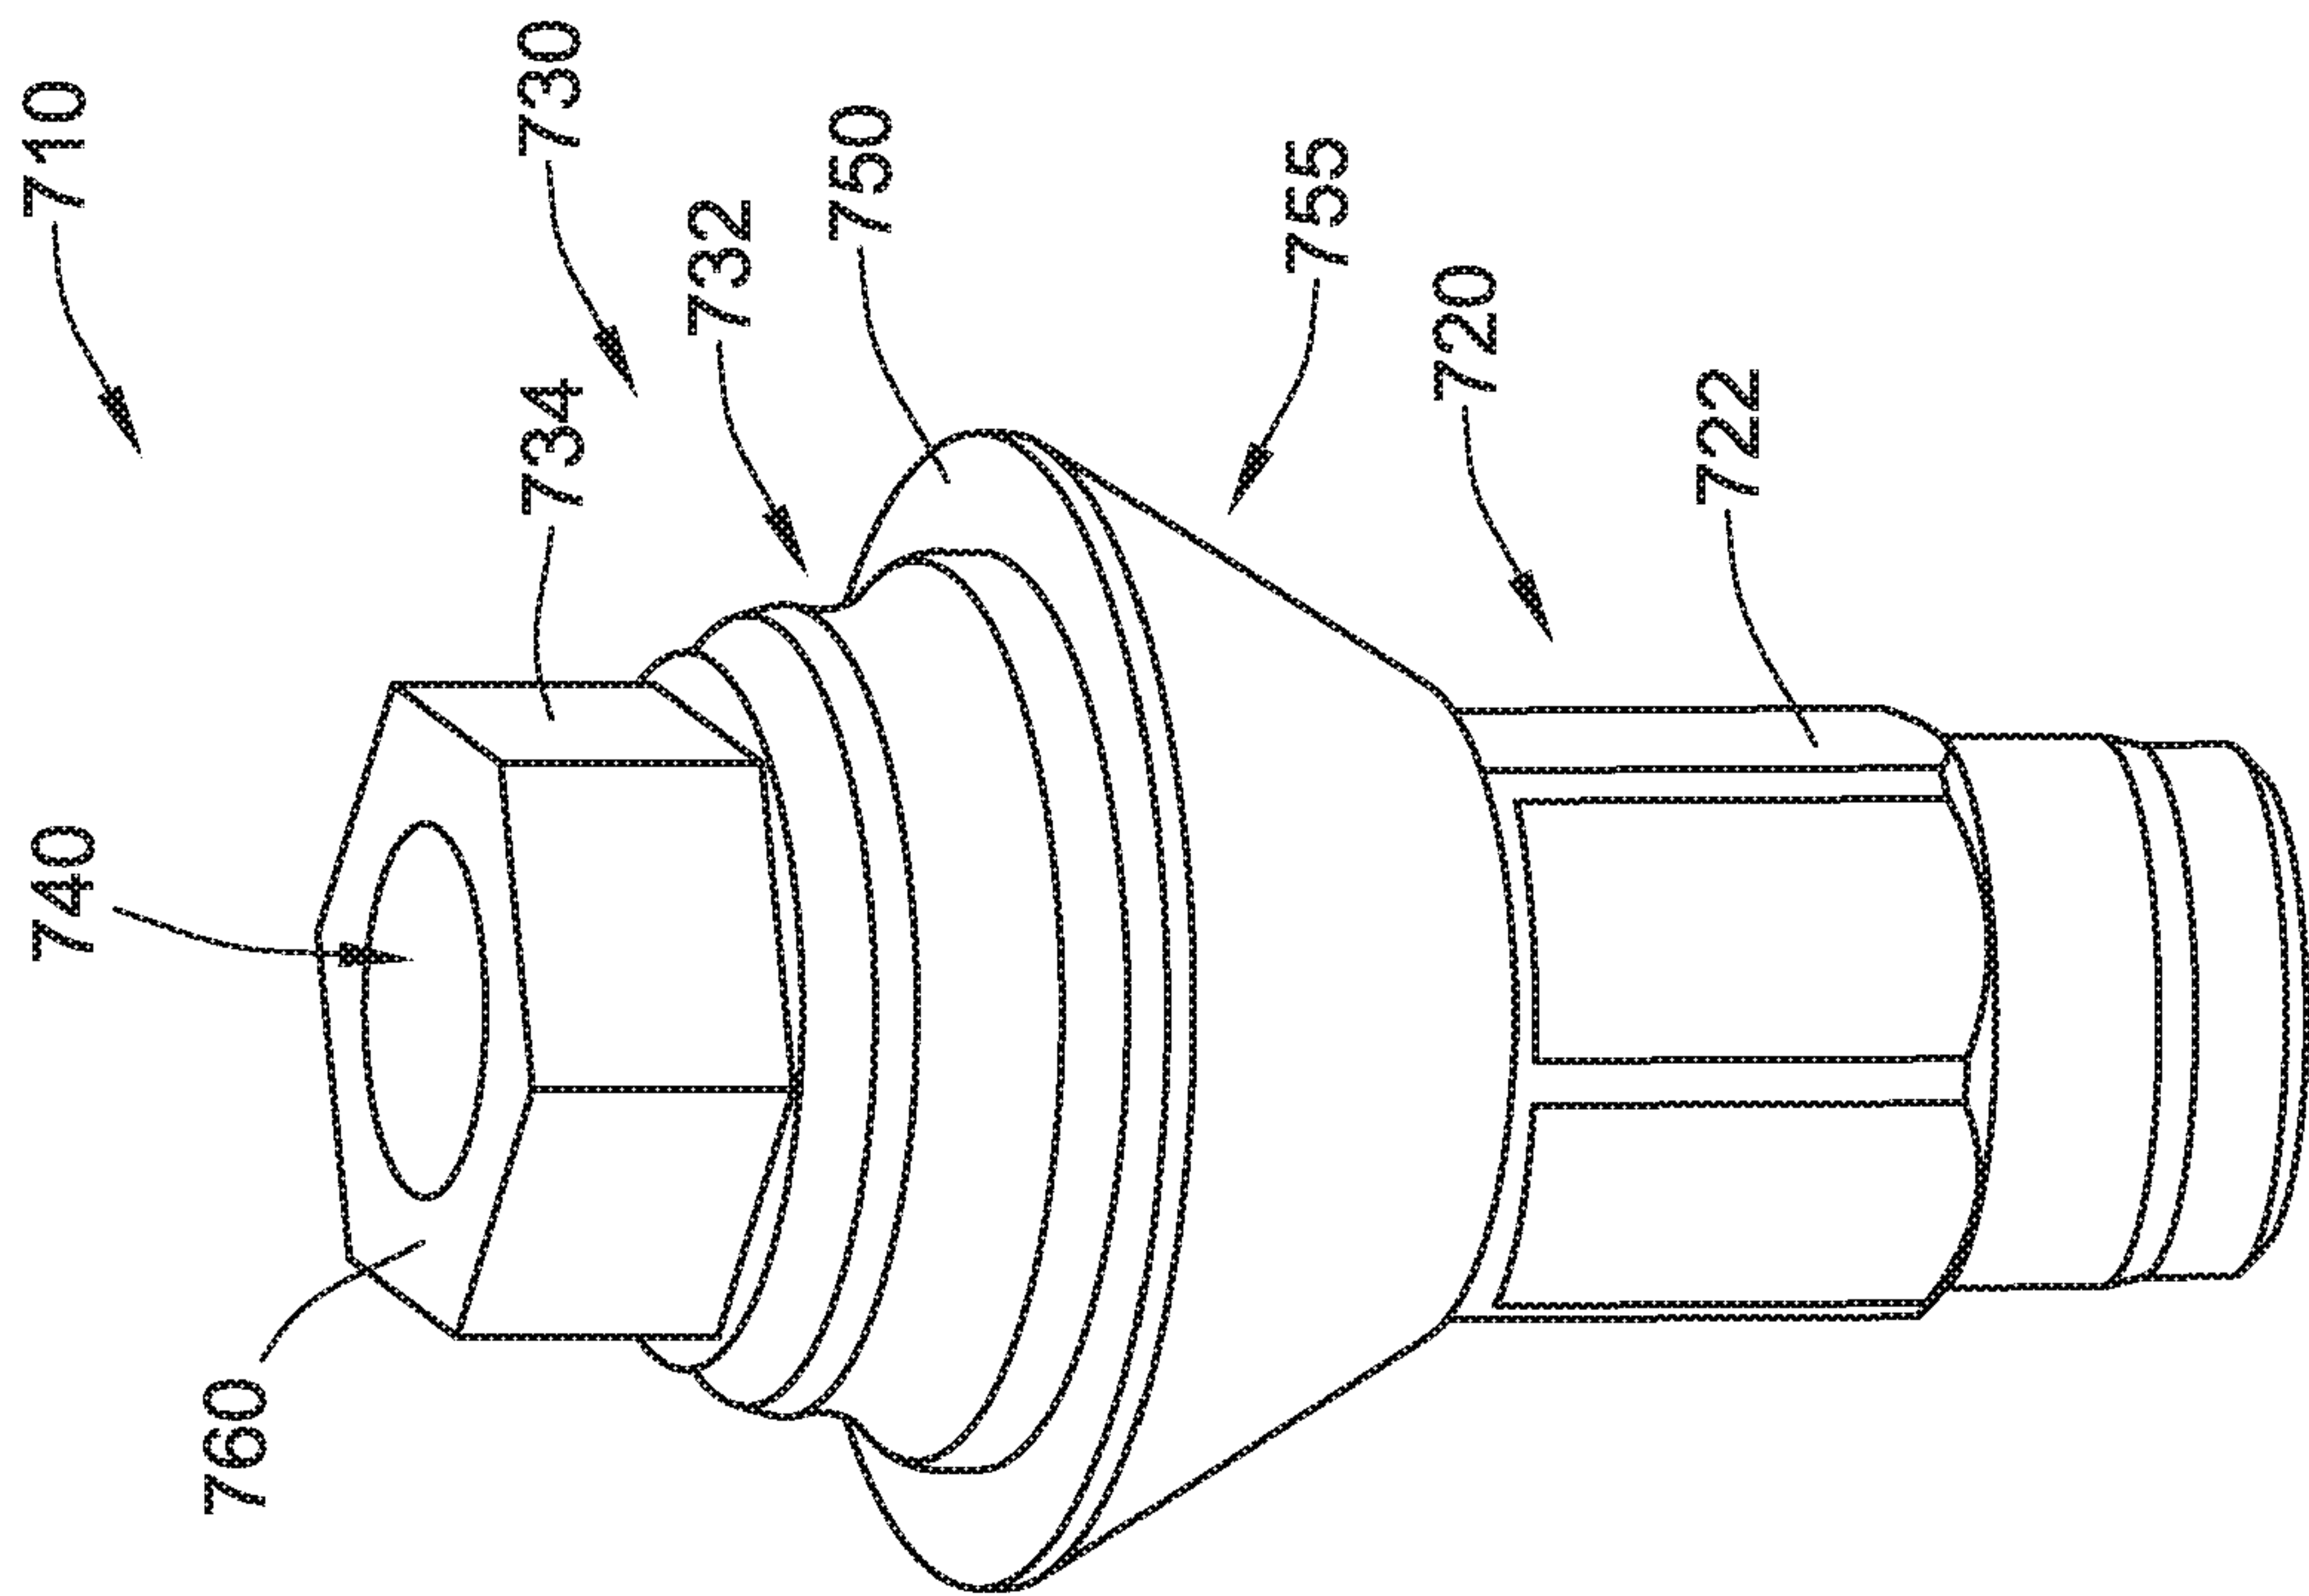


FIG. 11B

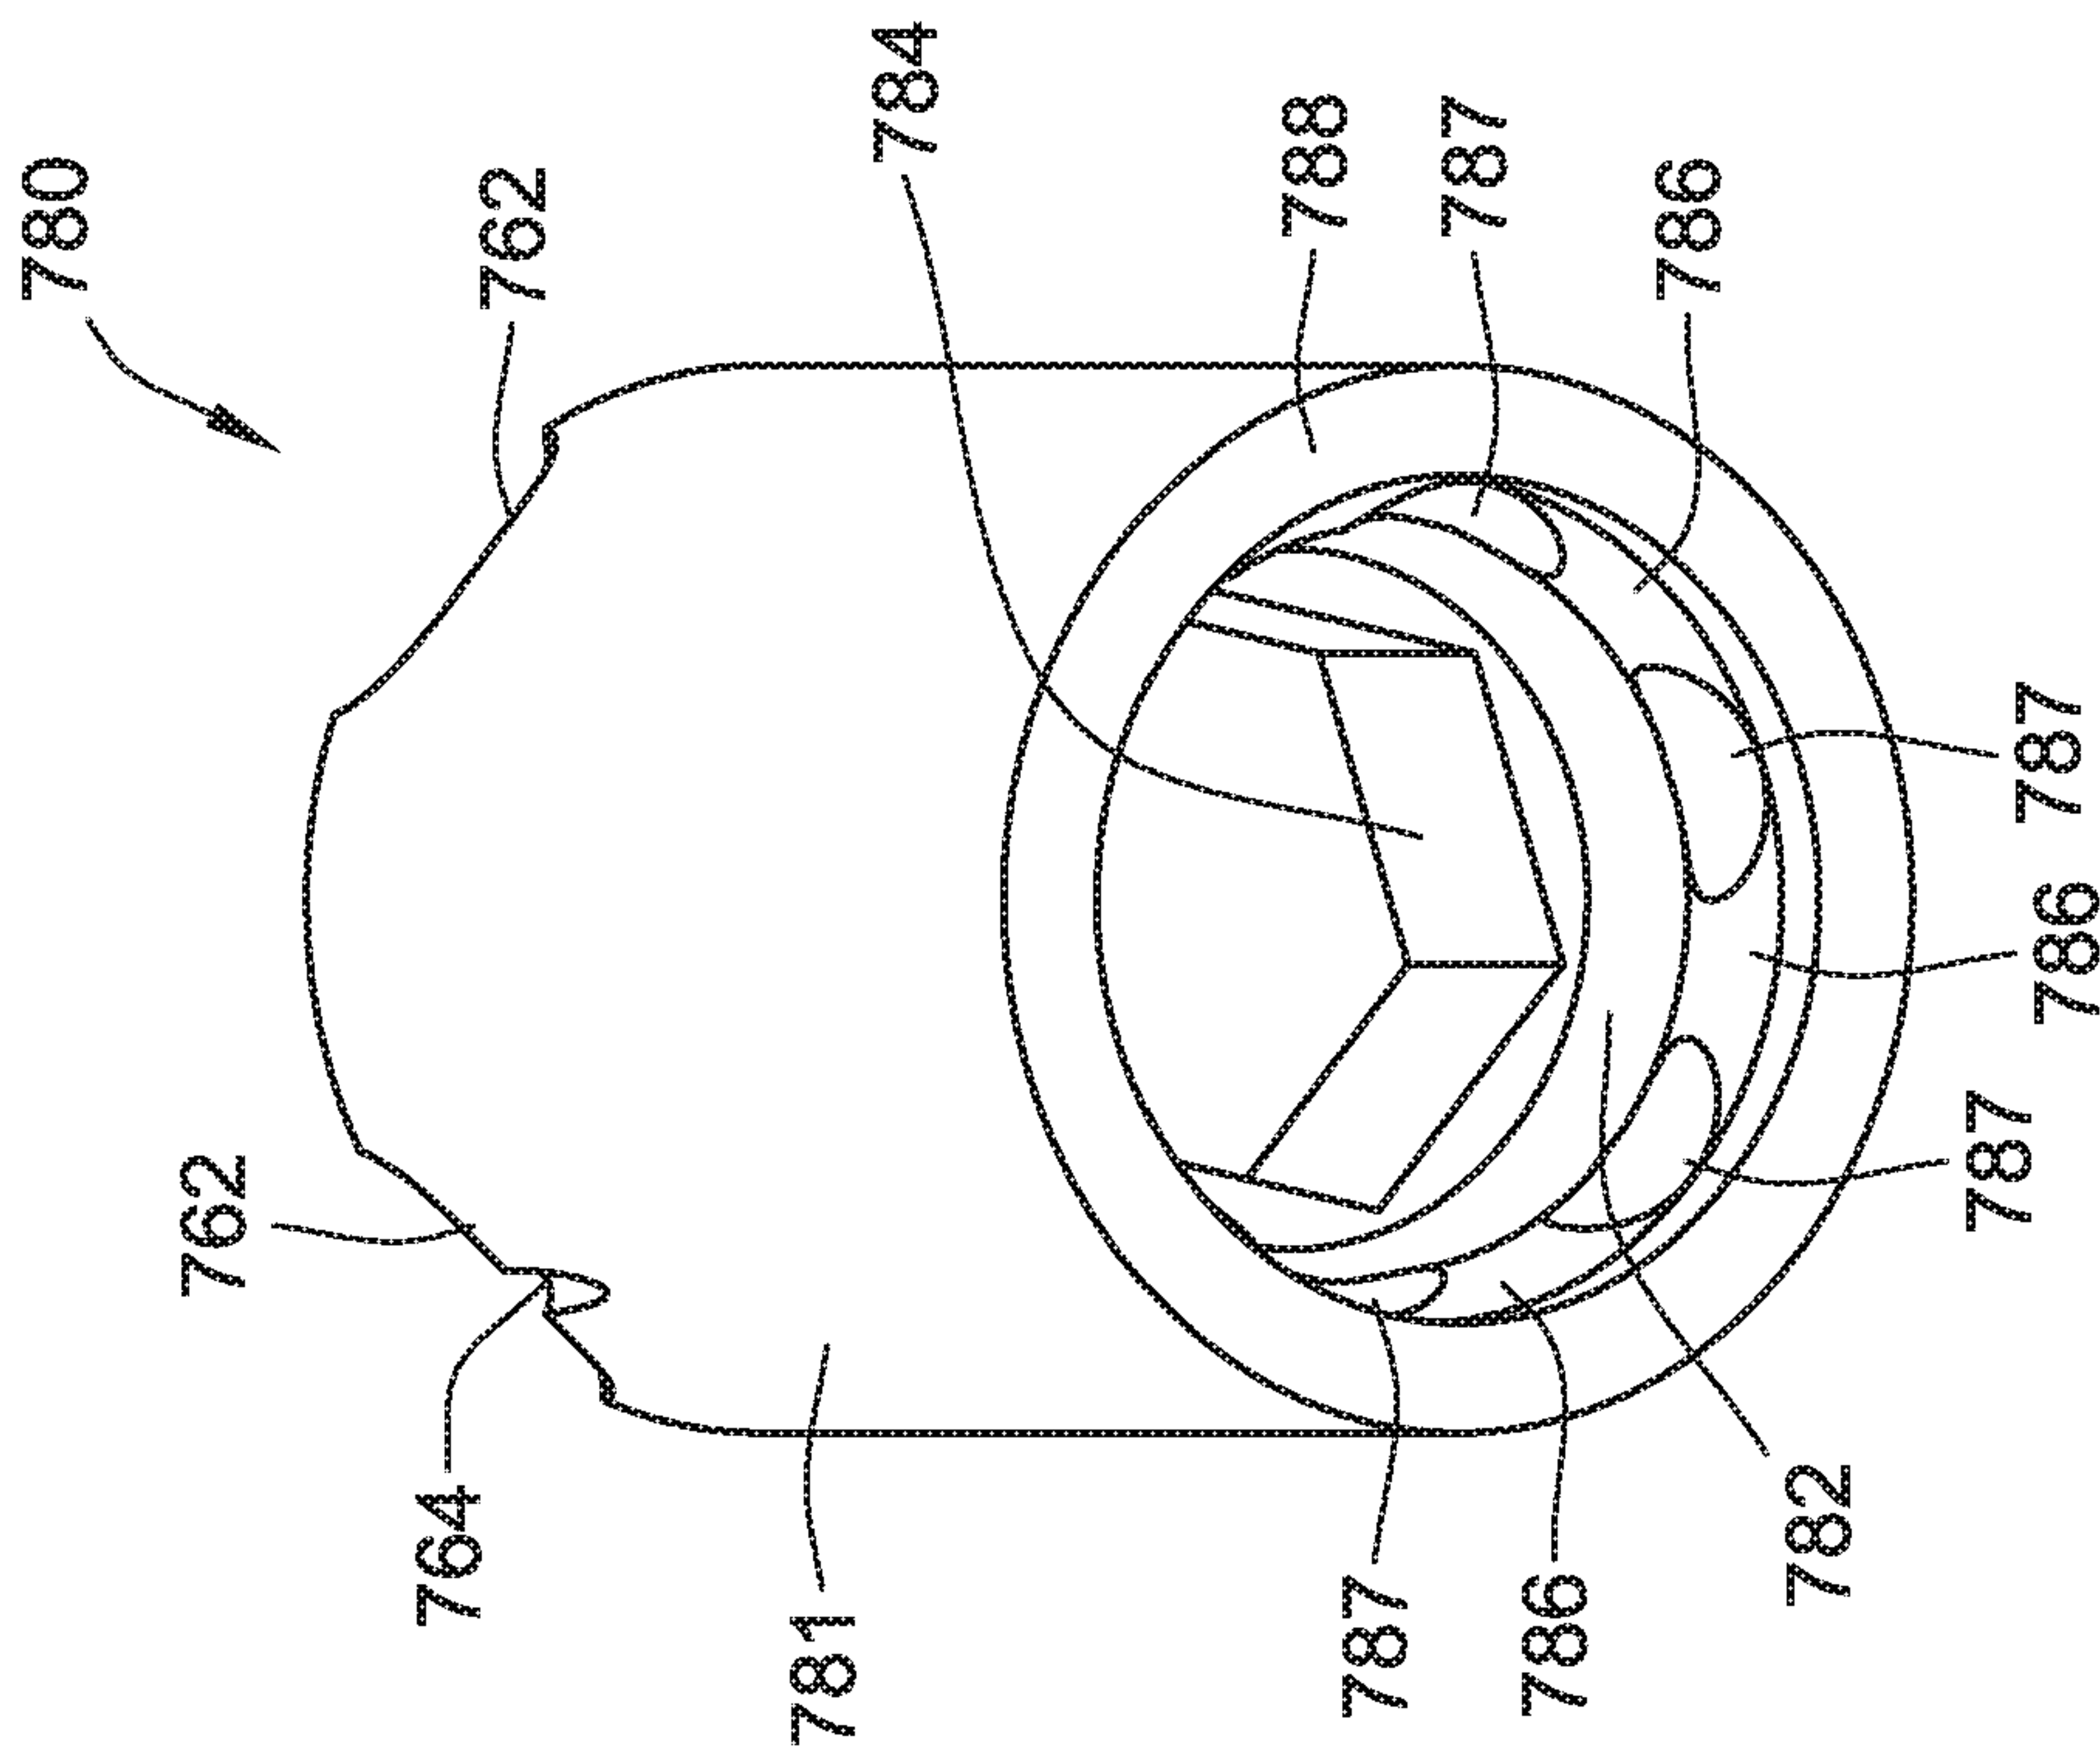


FIG. 11C

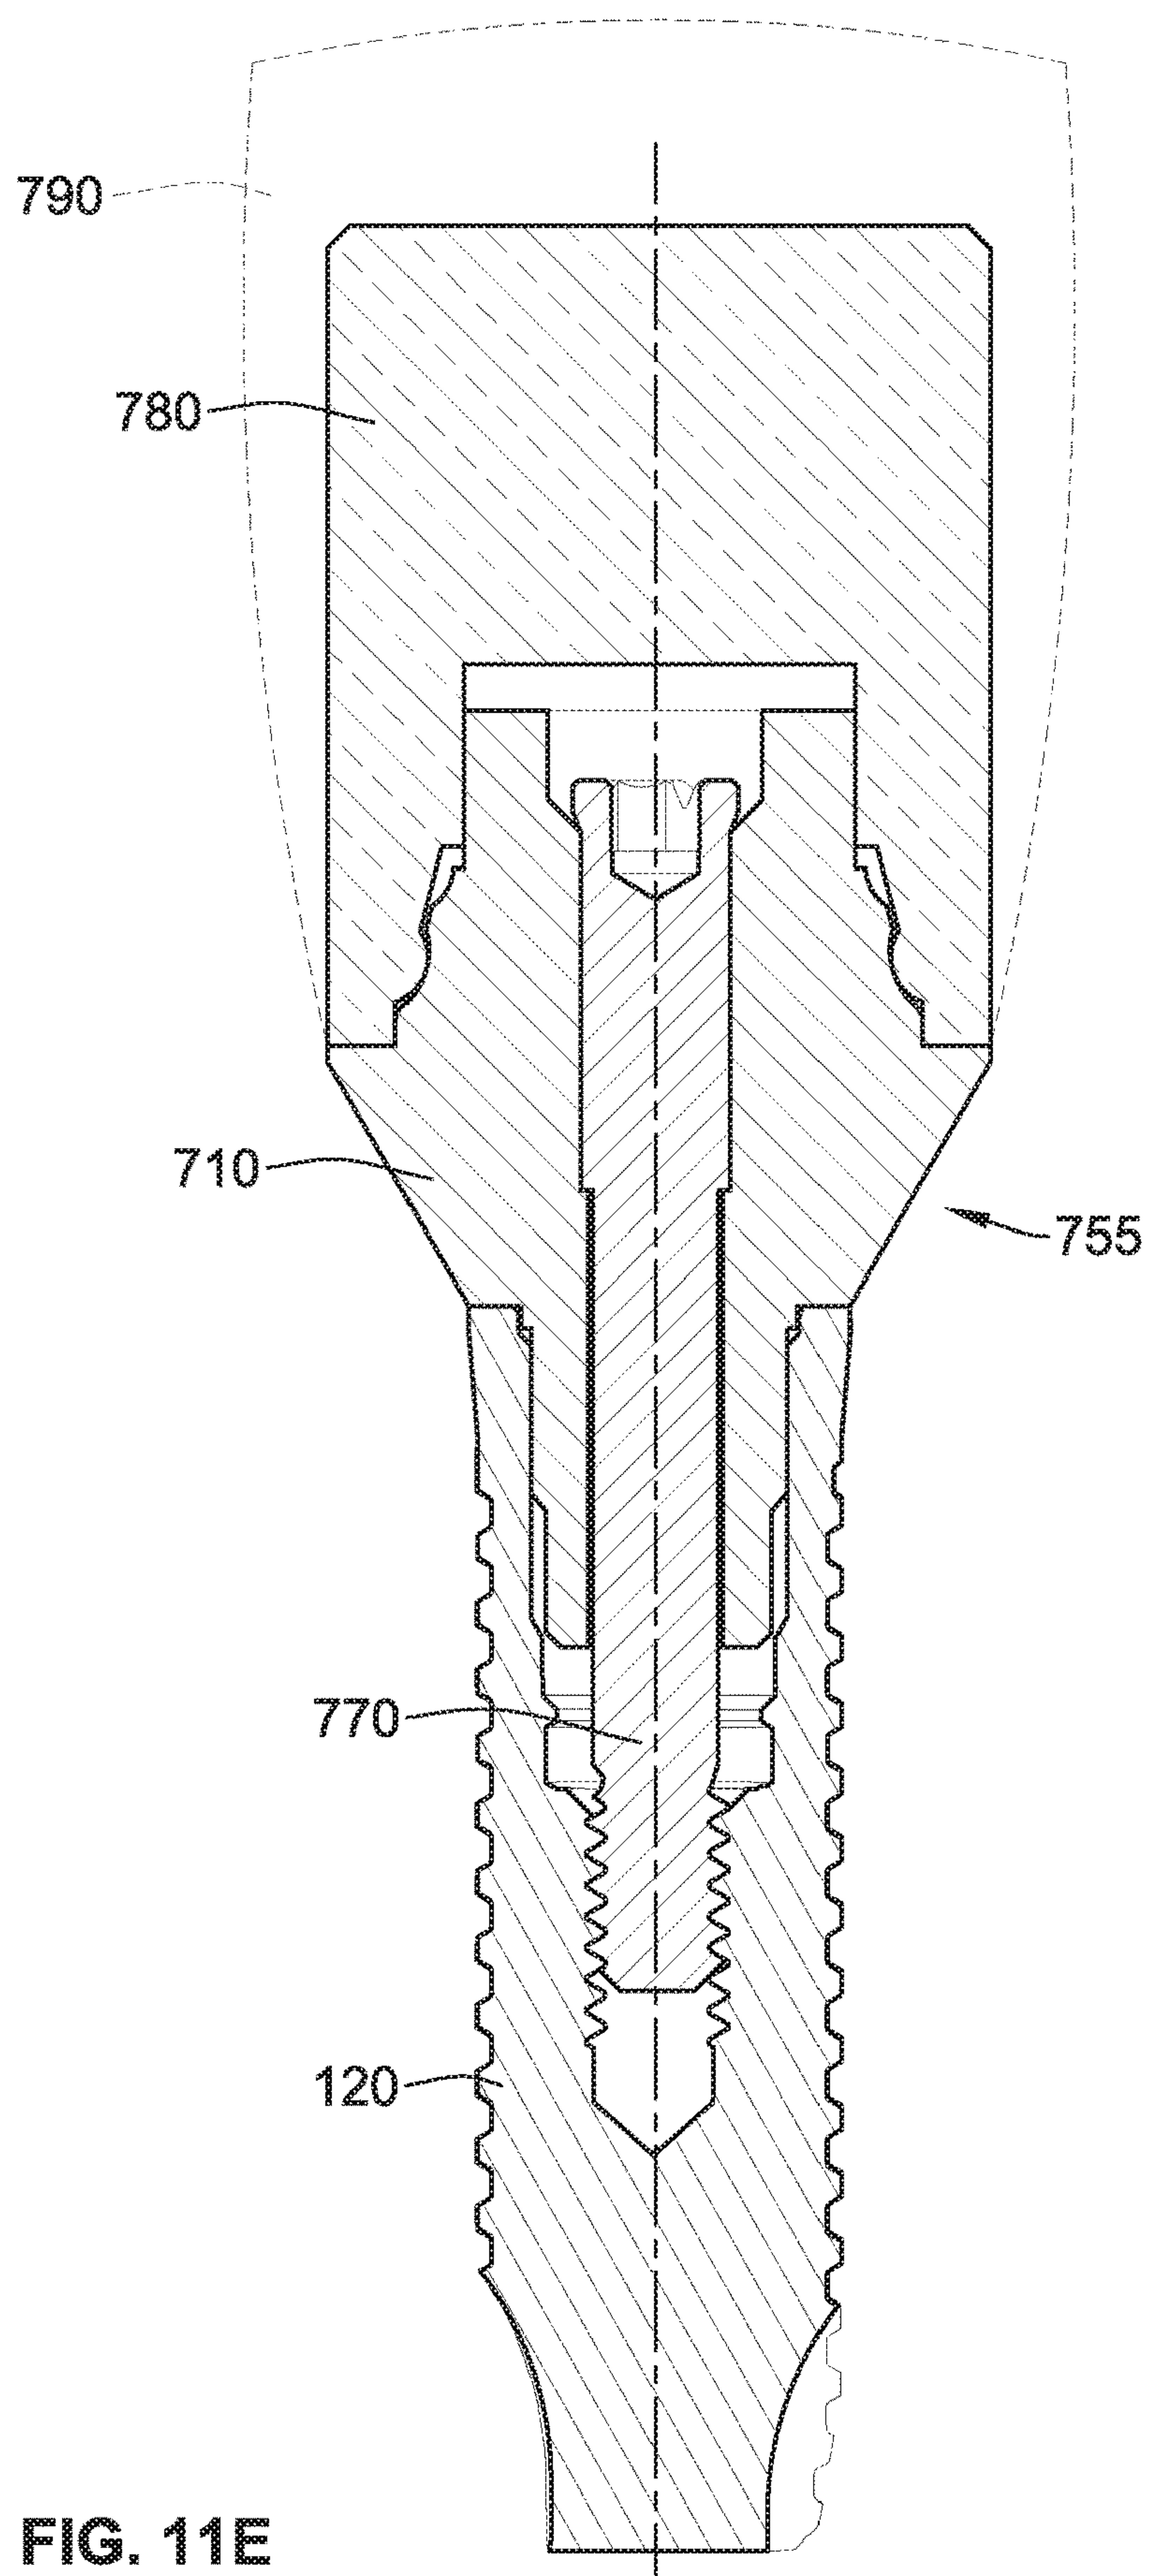
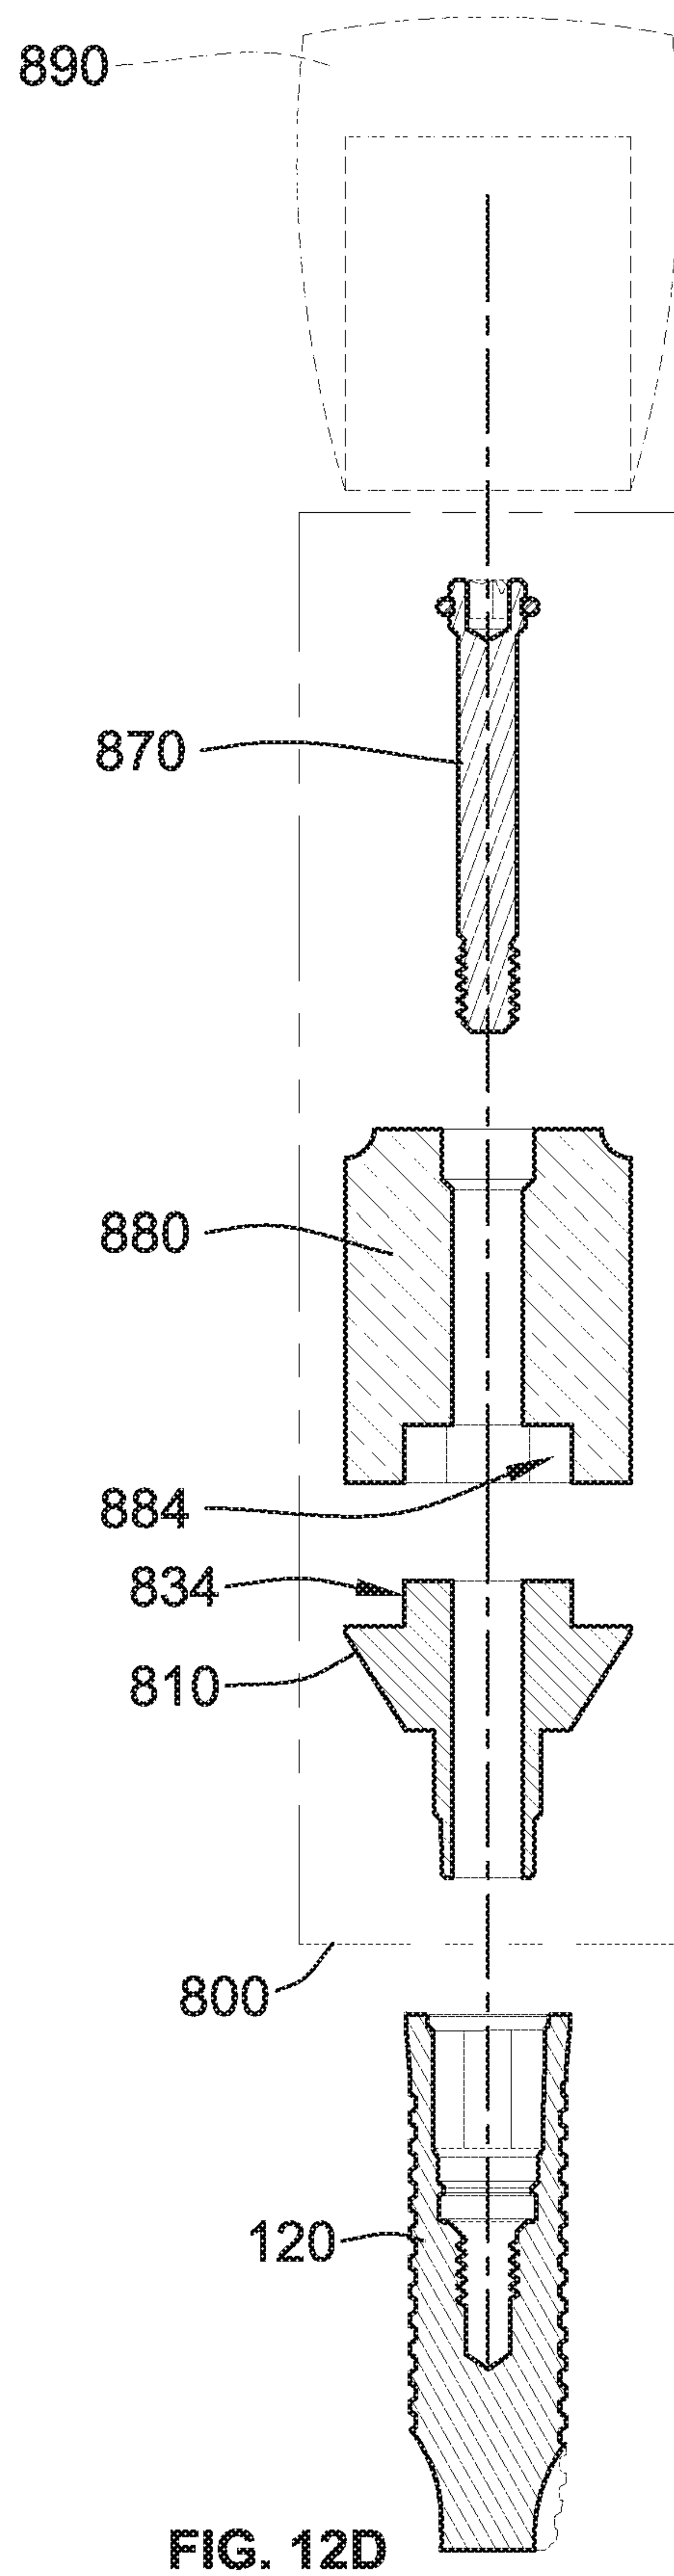
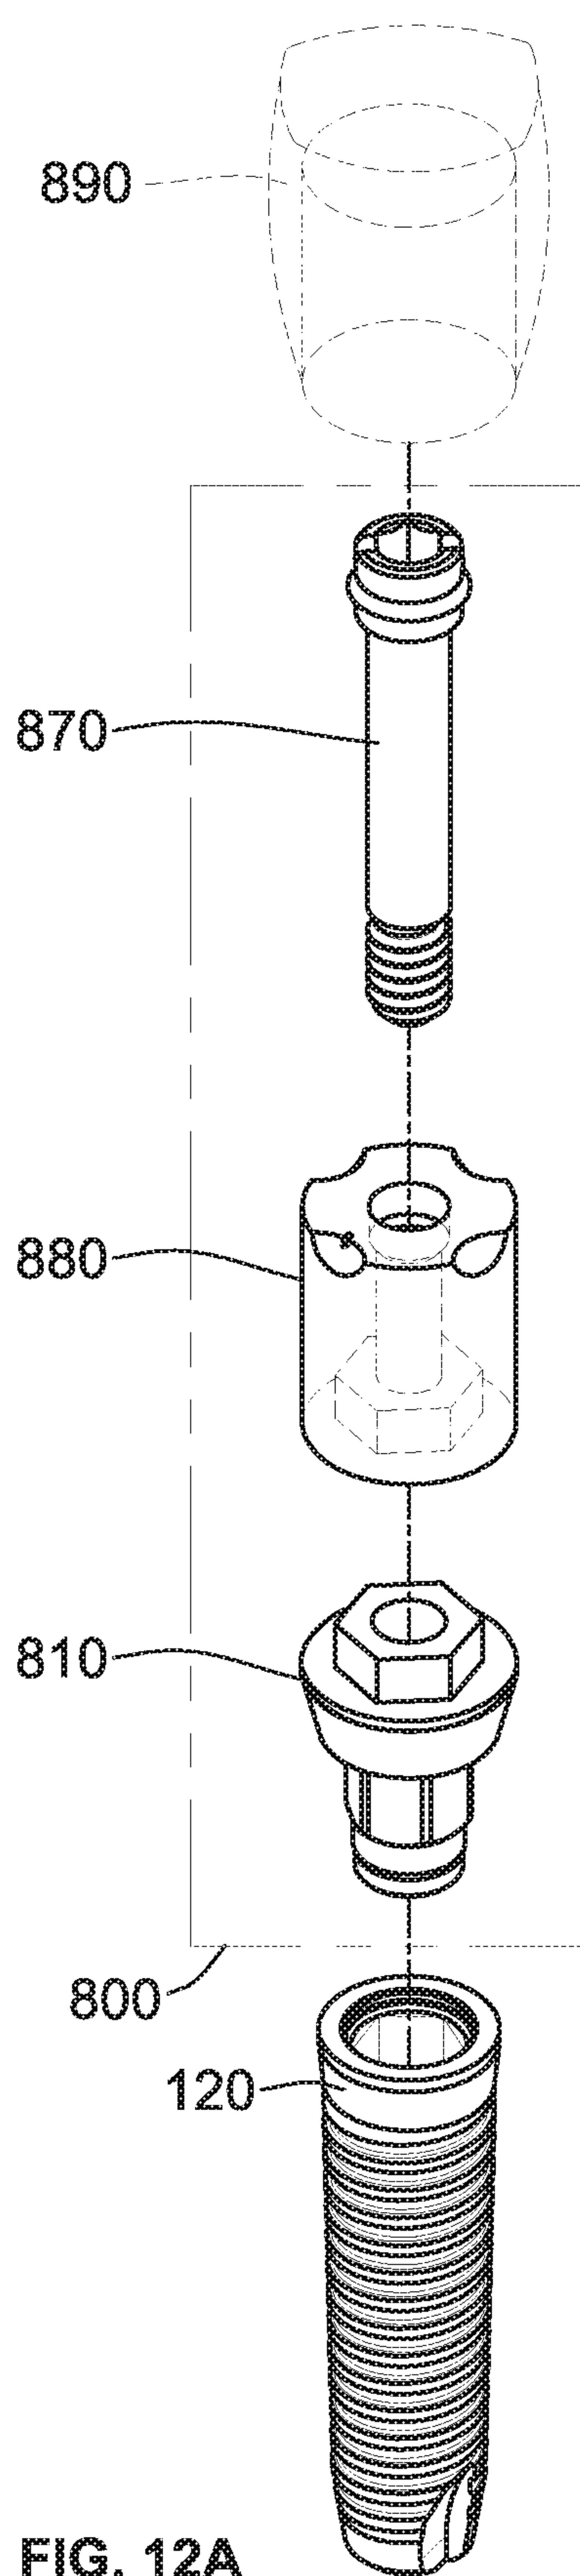


FIG. 11E





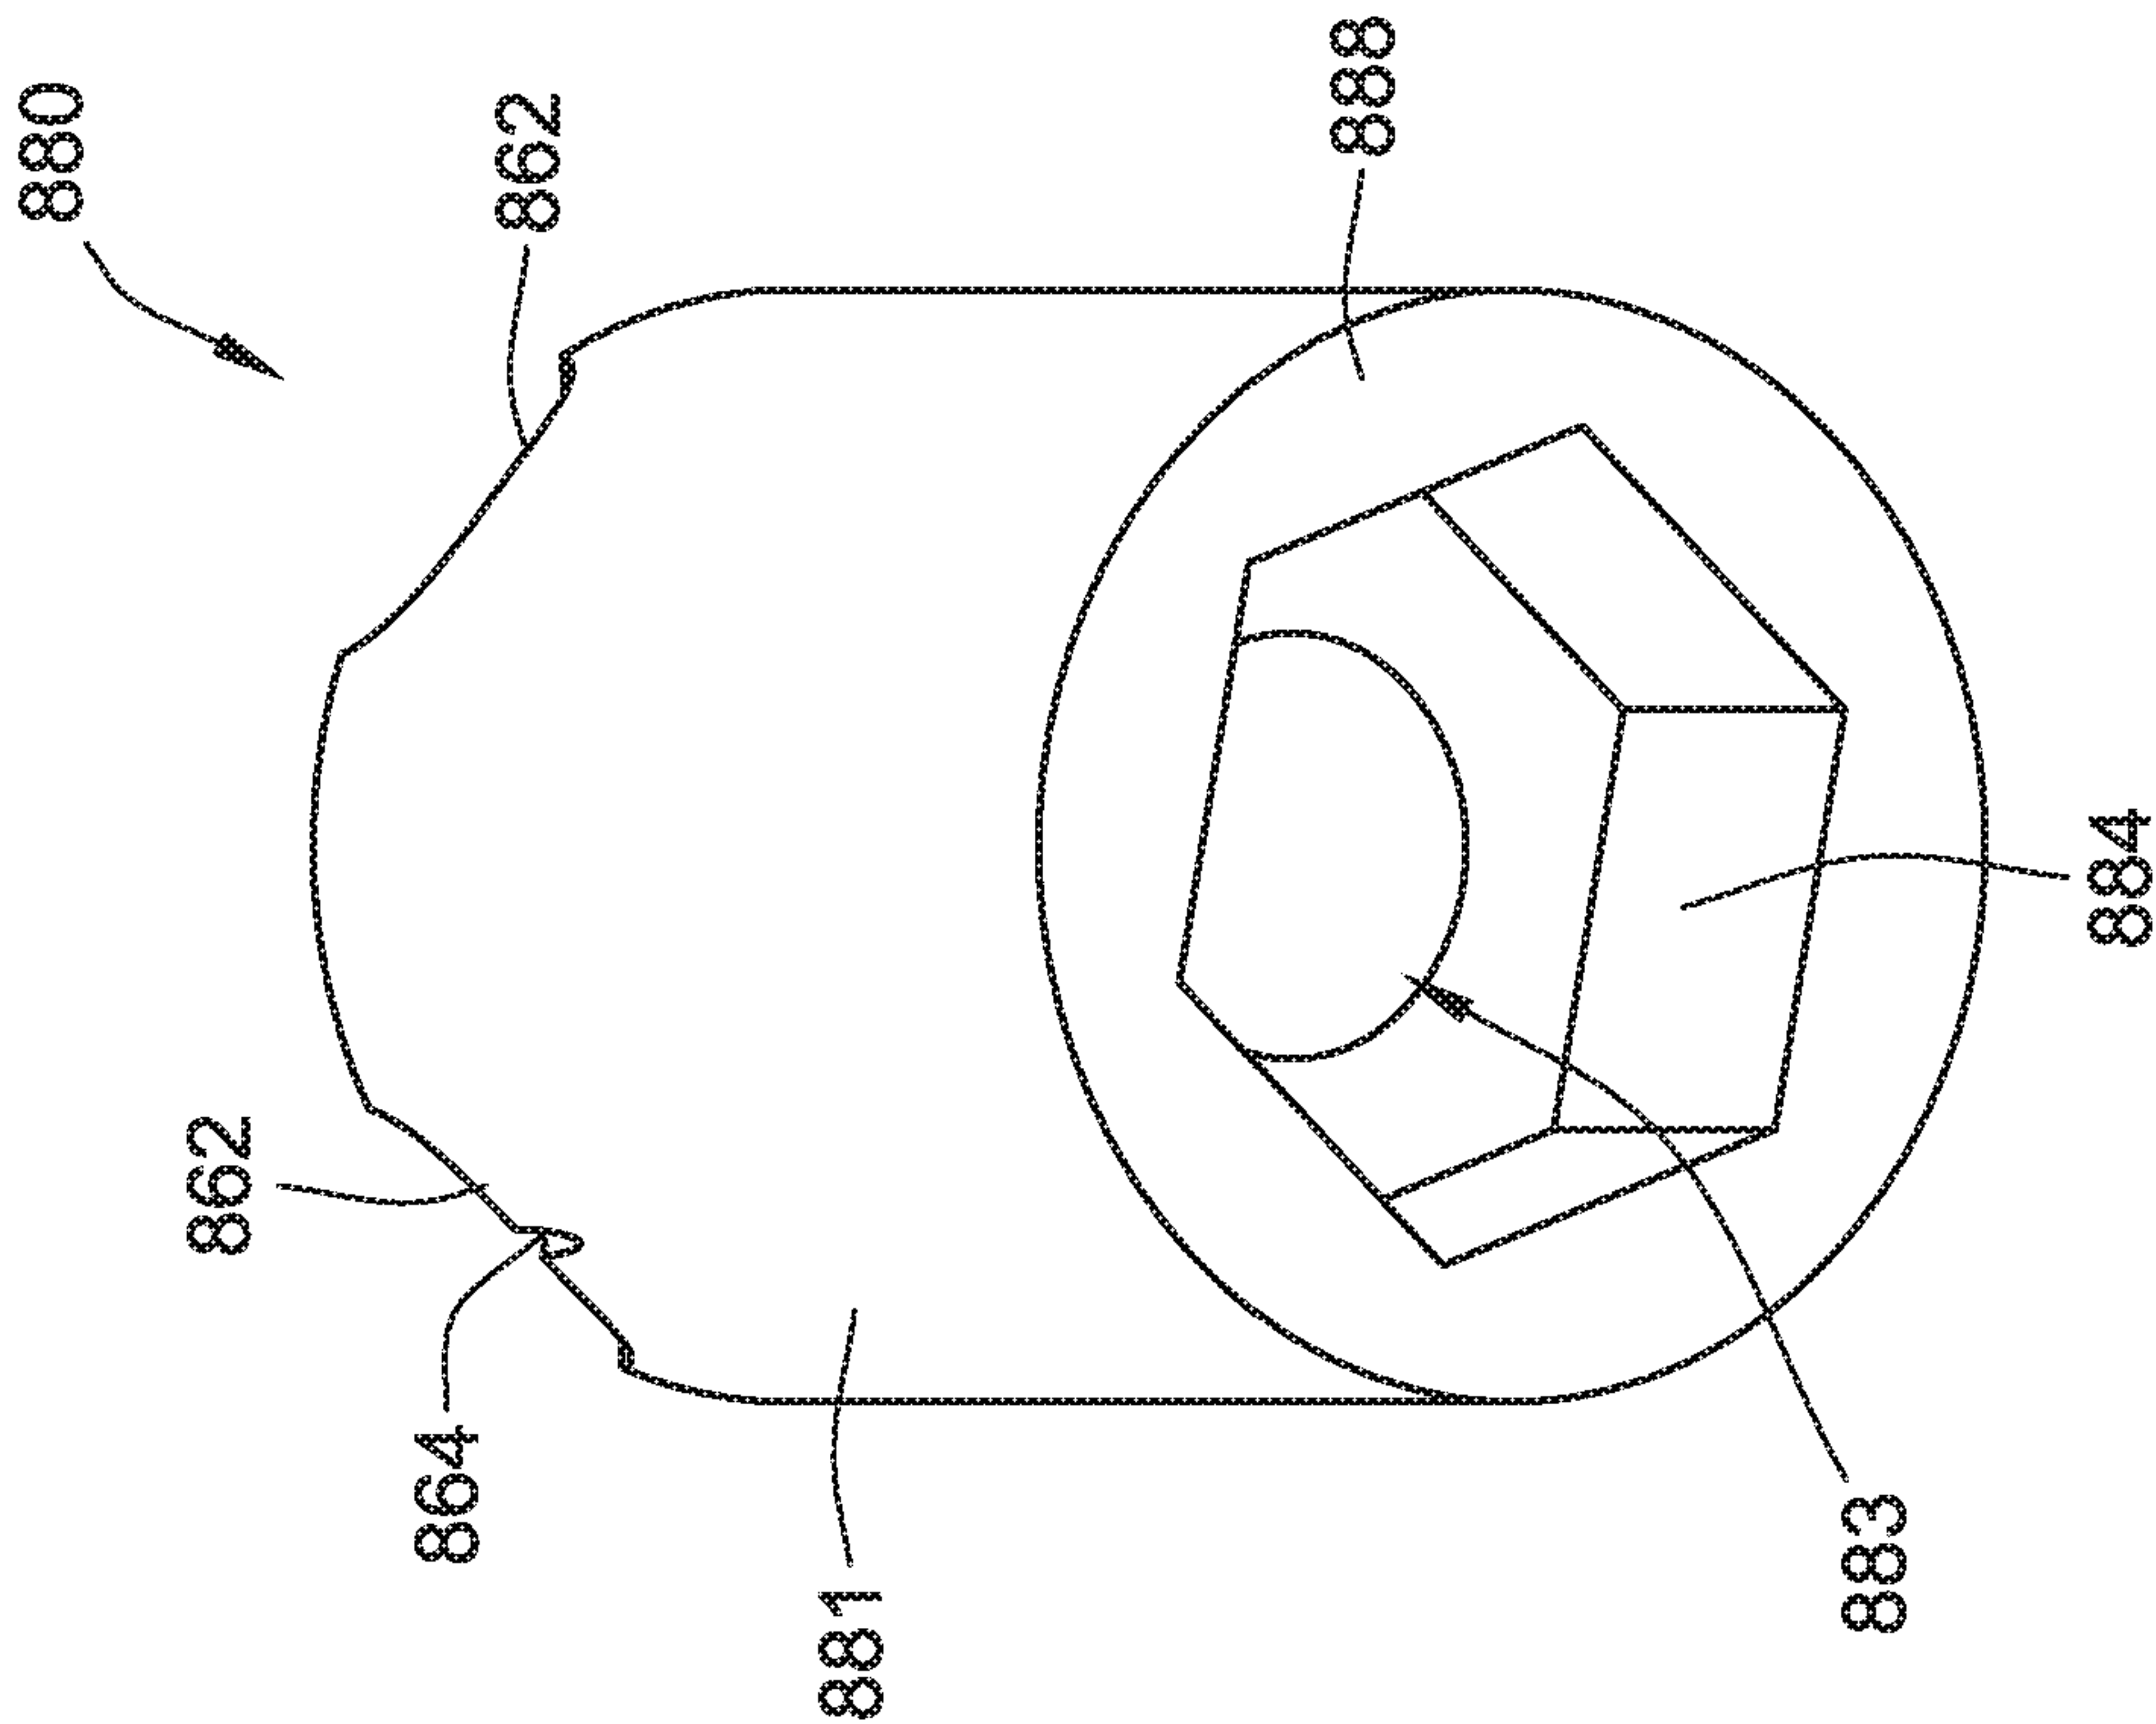


FIG. 12C

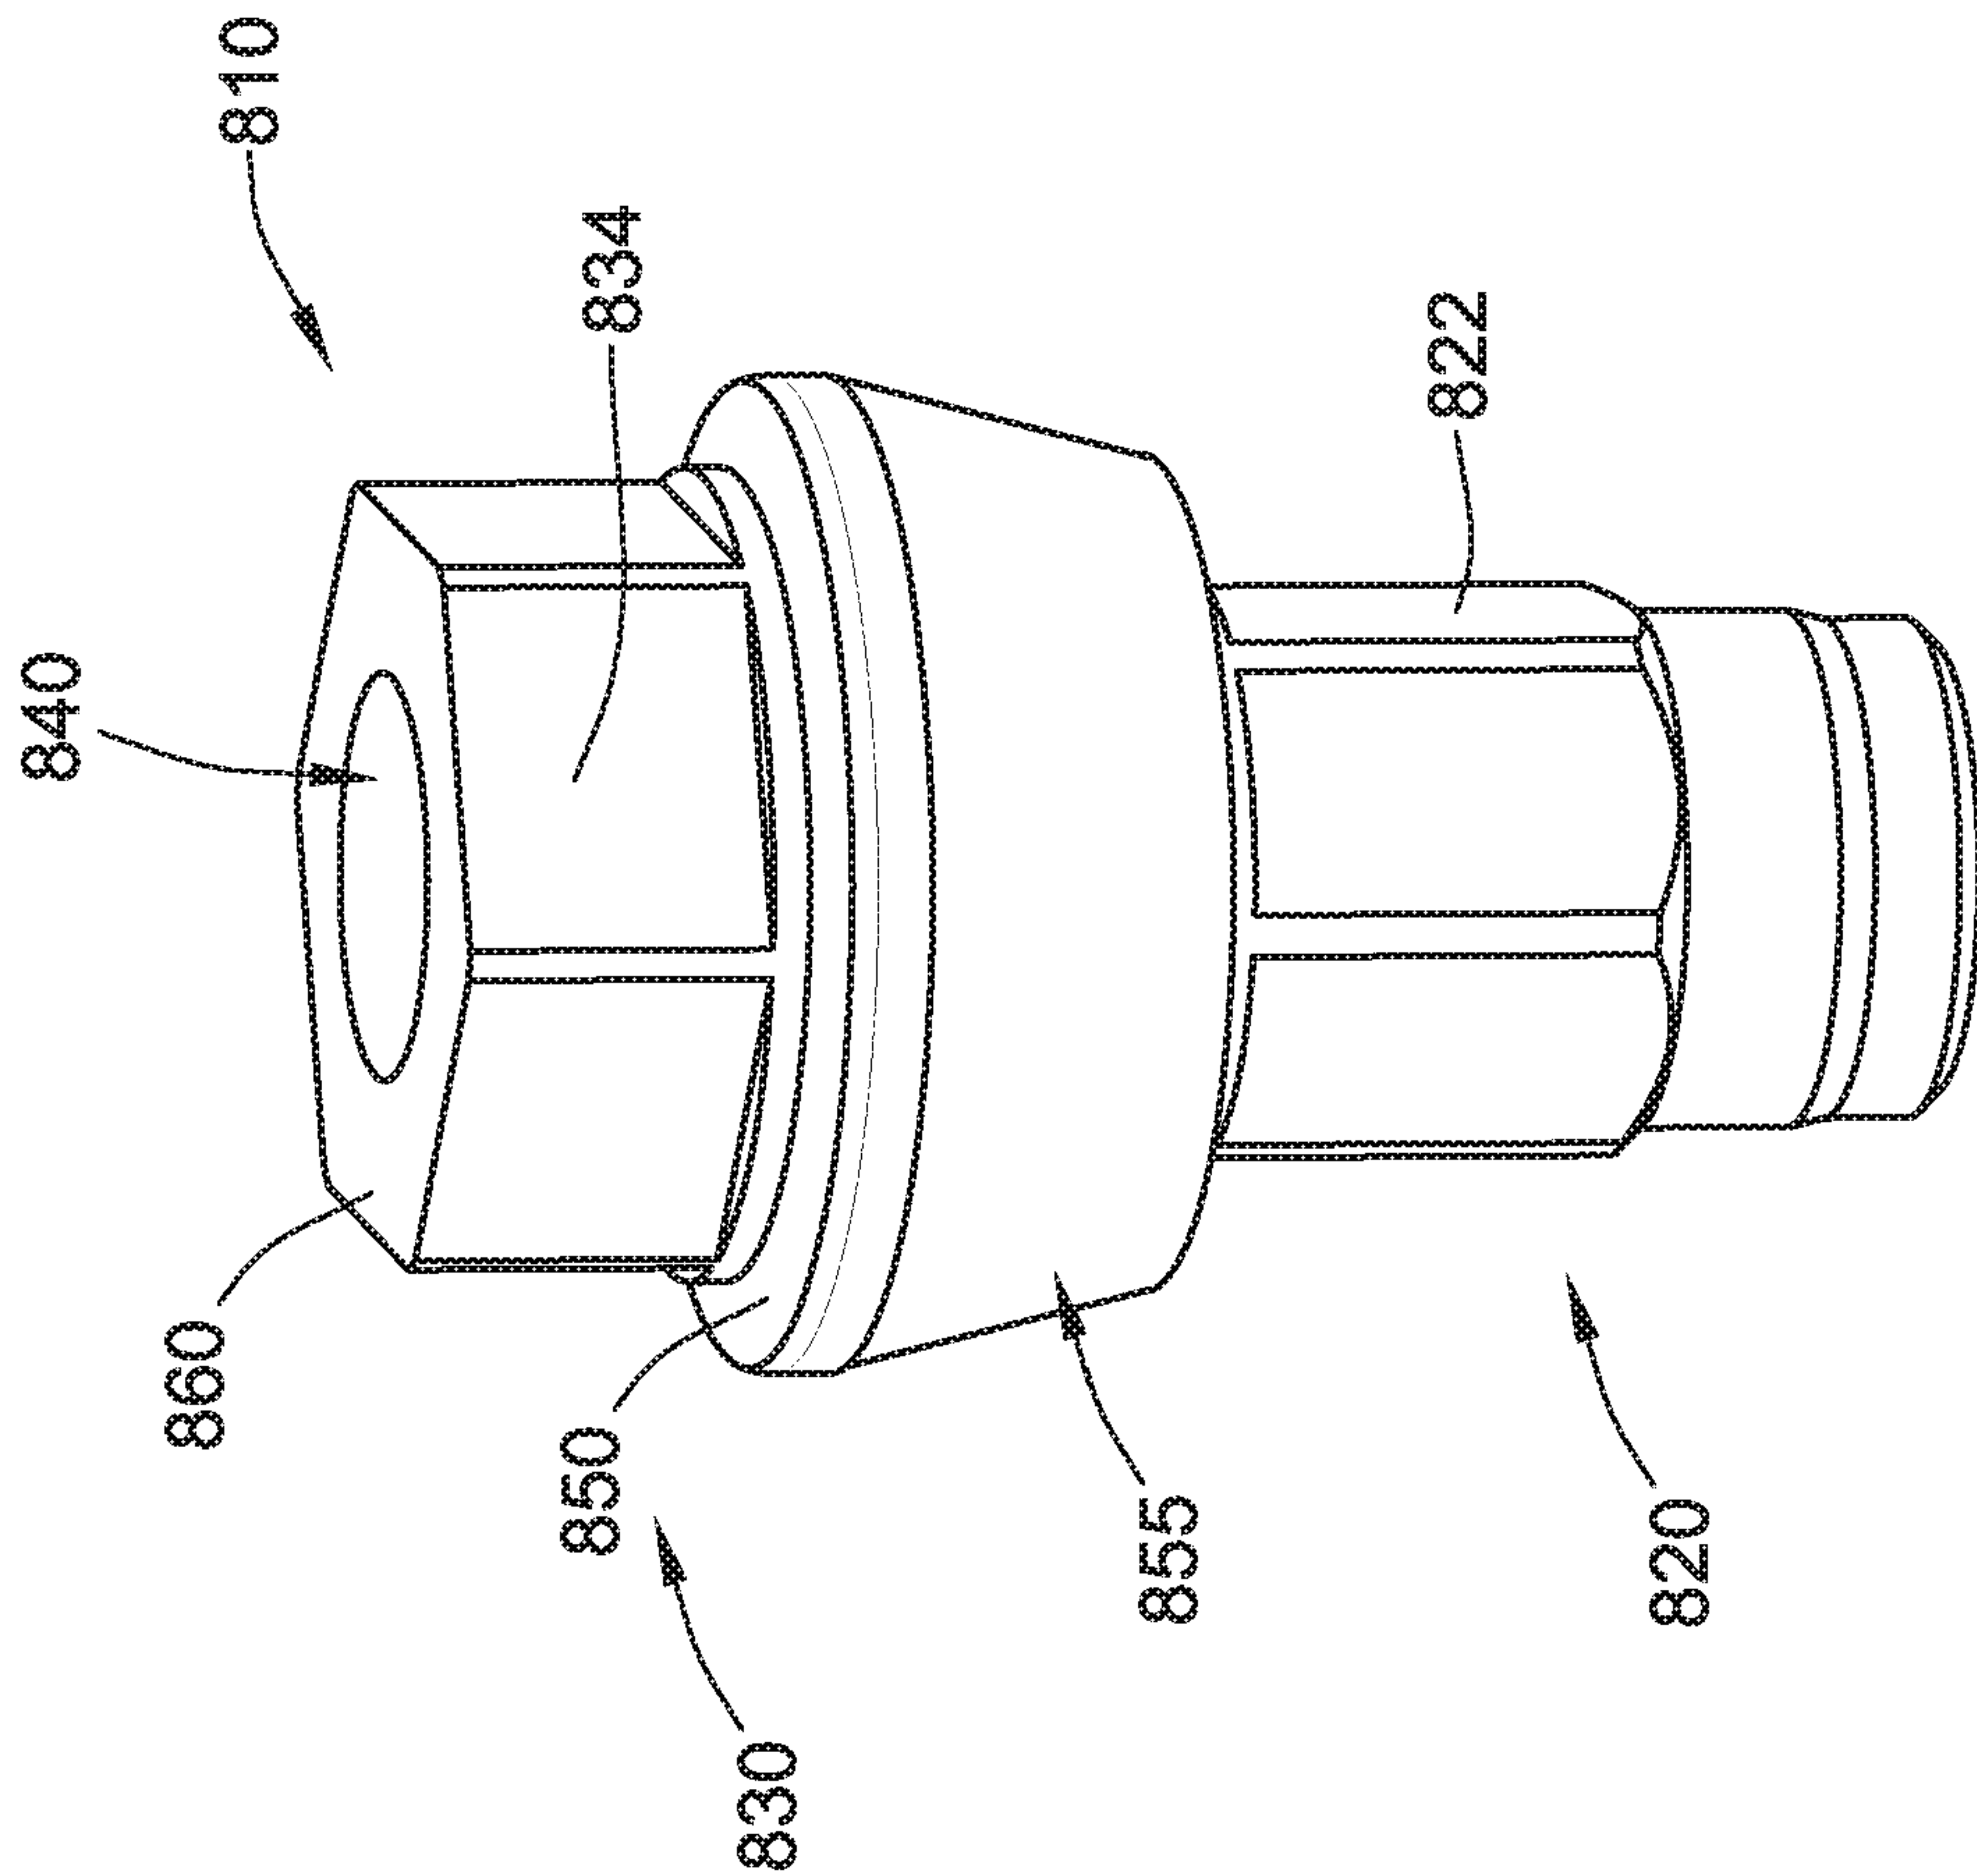


FIG. 12B



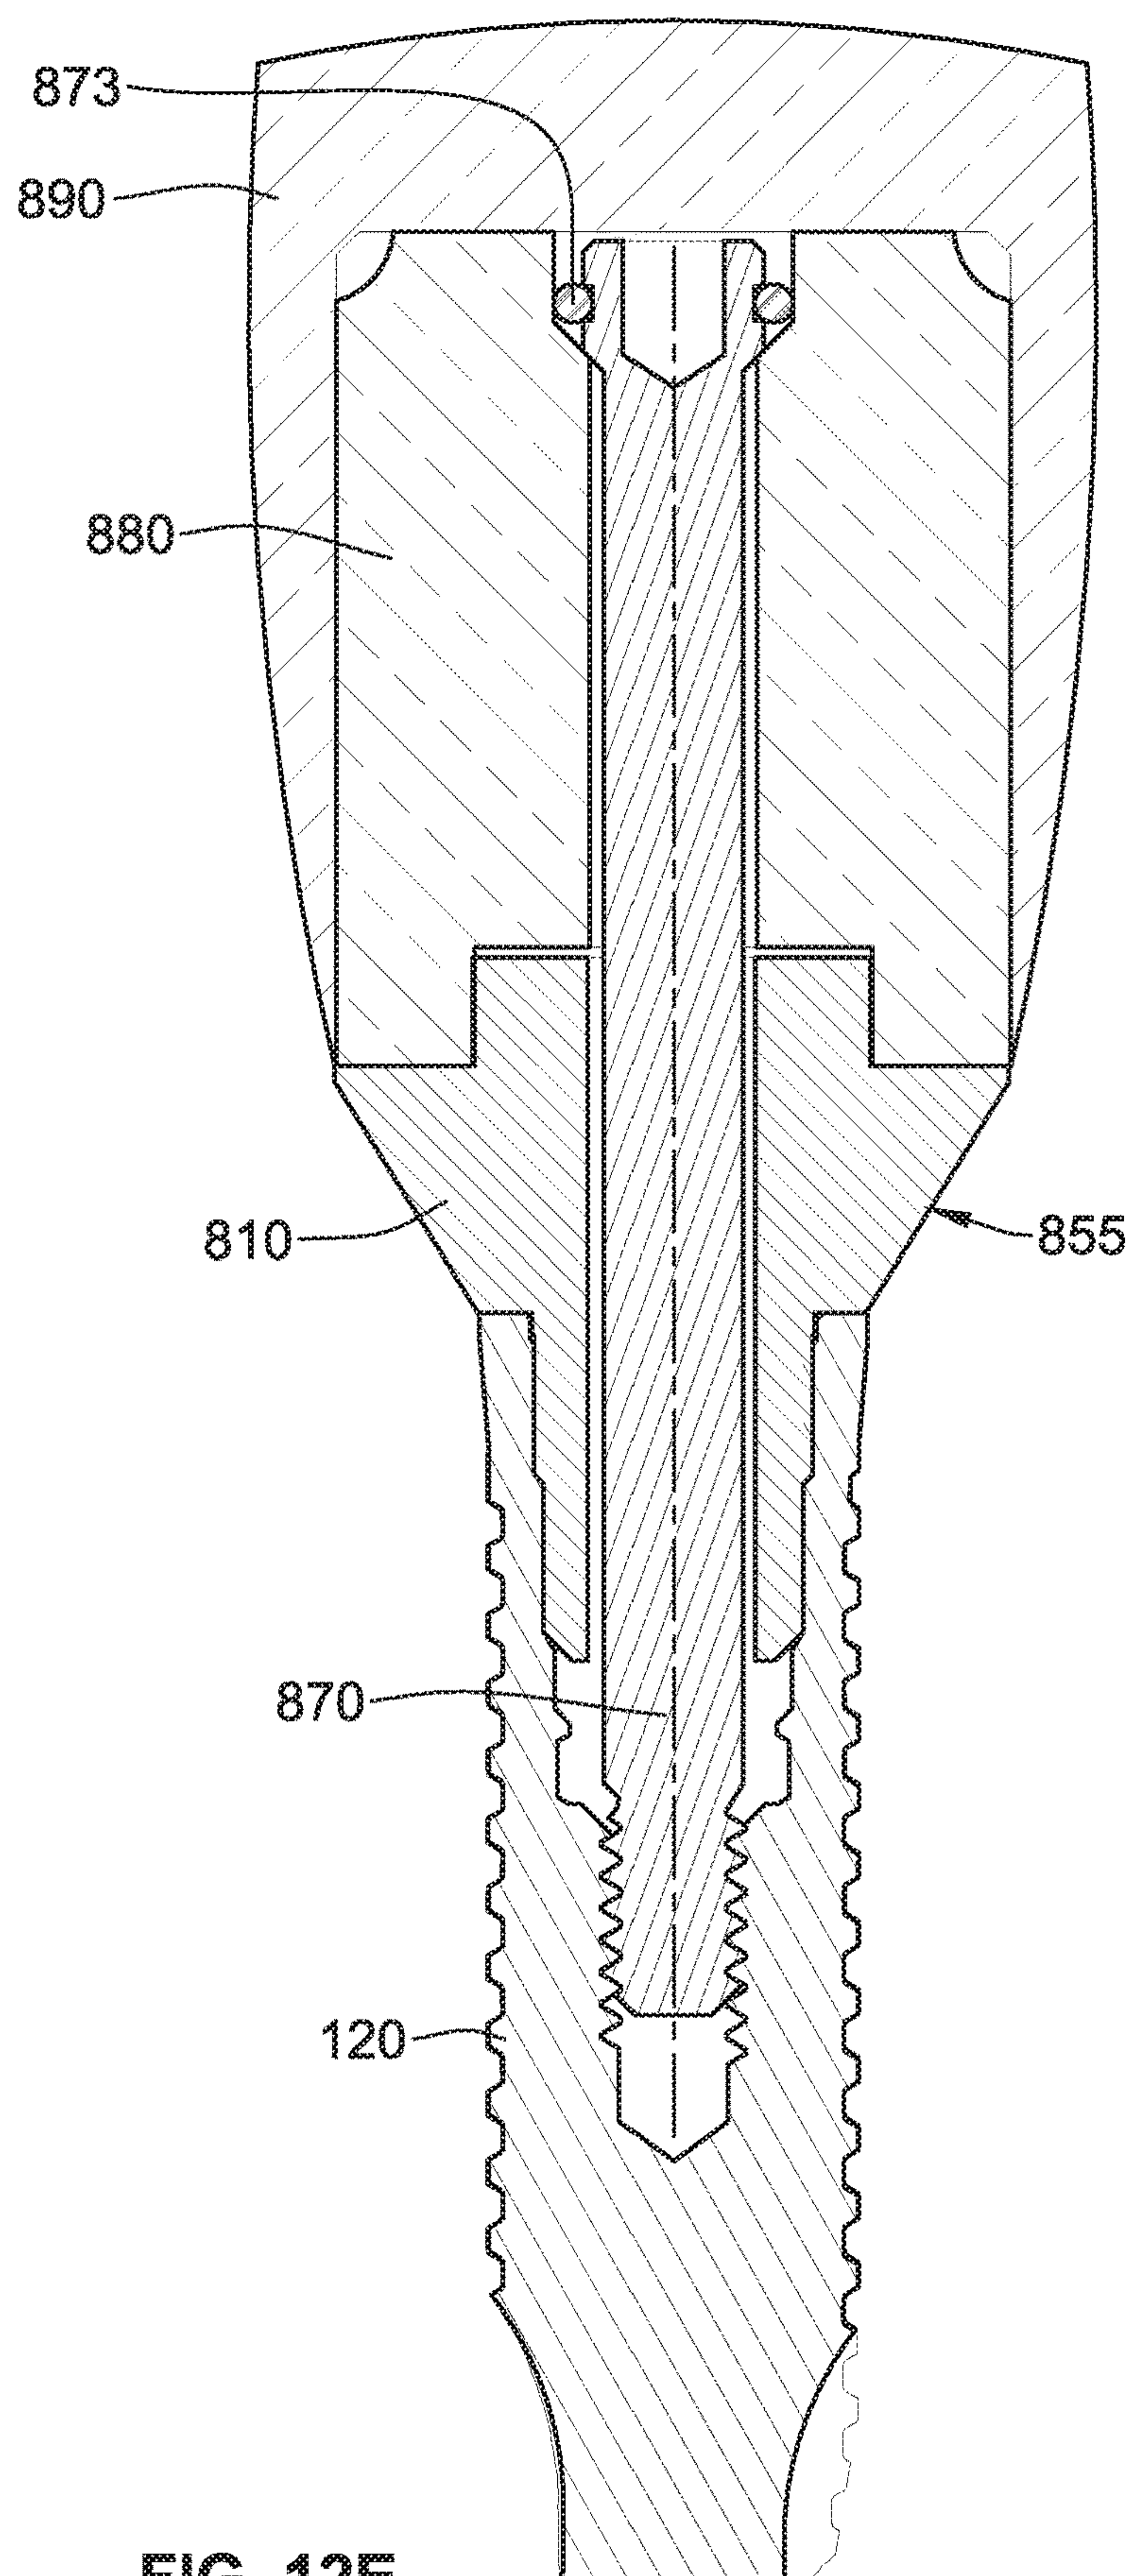


FIG. 12E

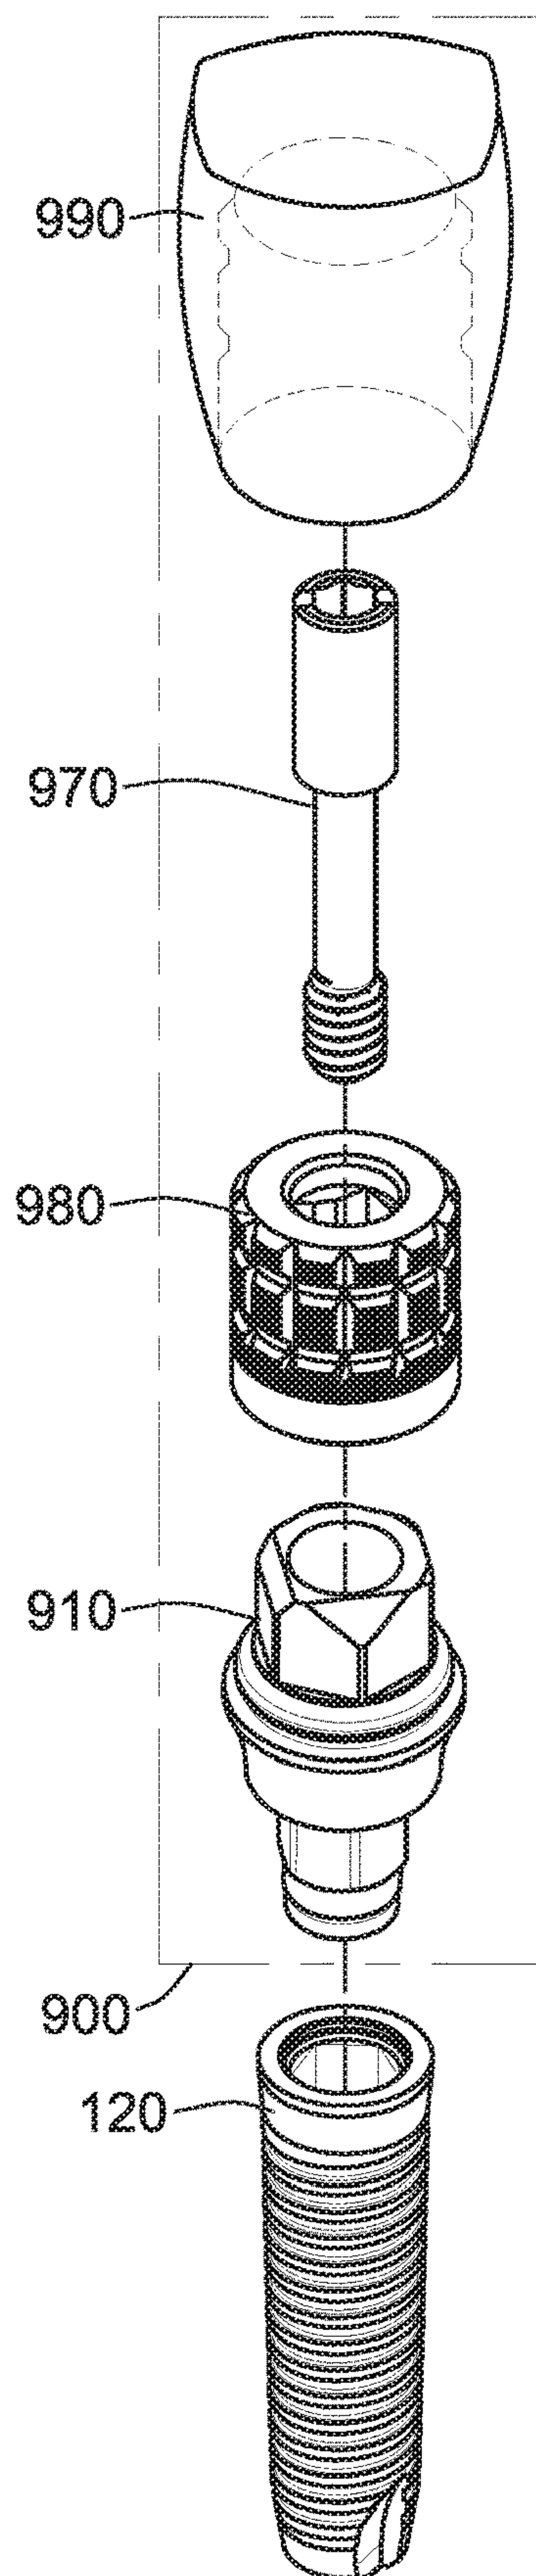


FIG. 13A

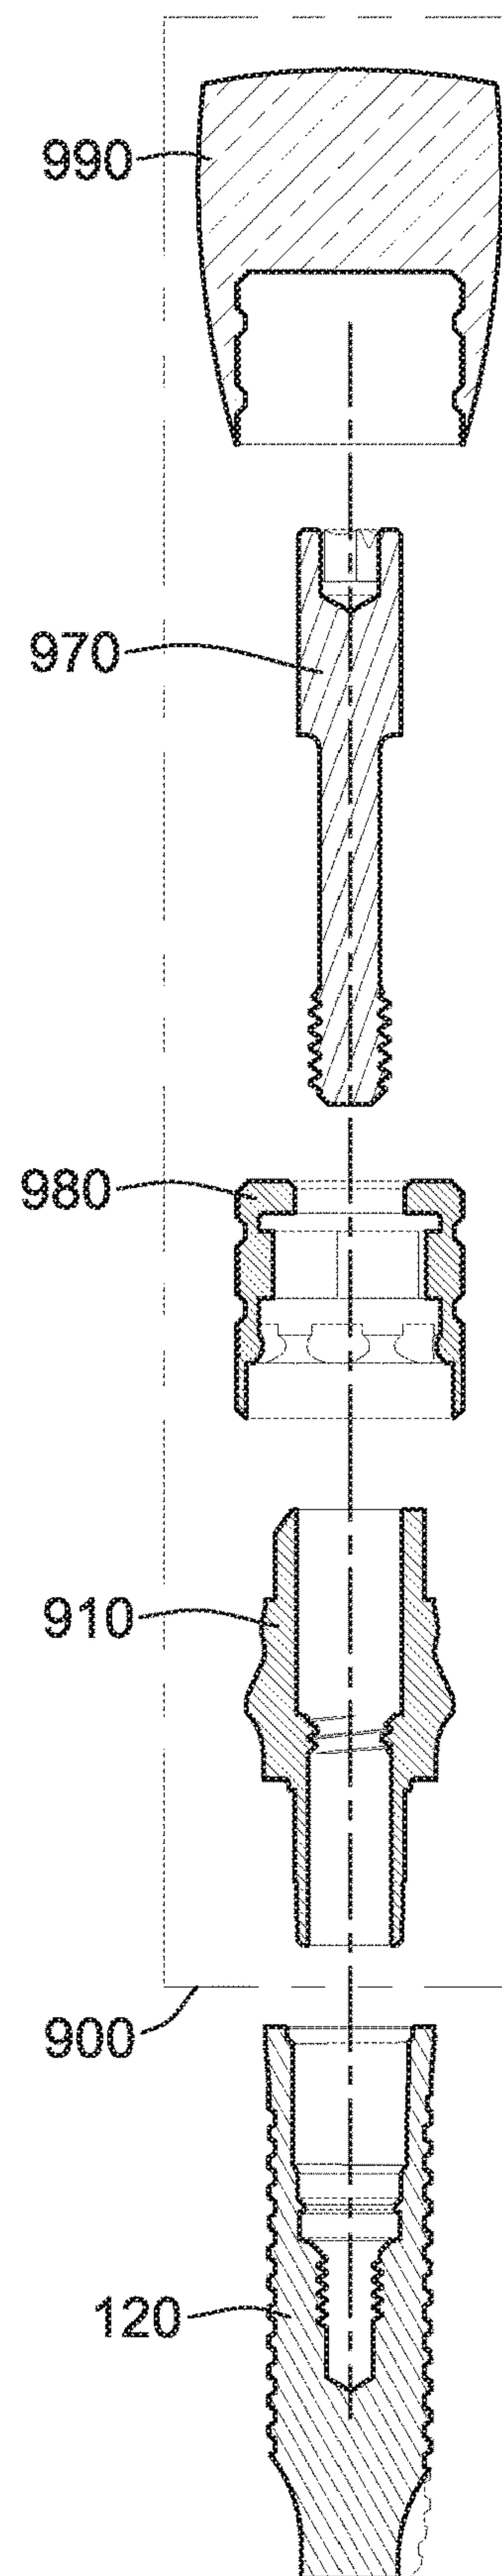
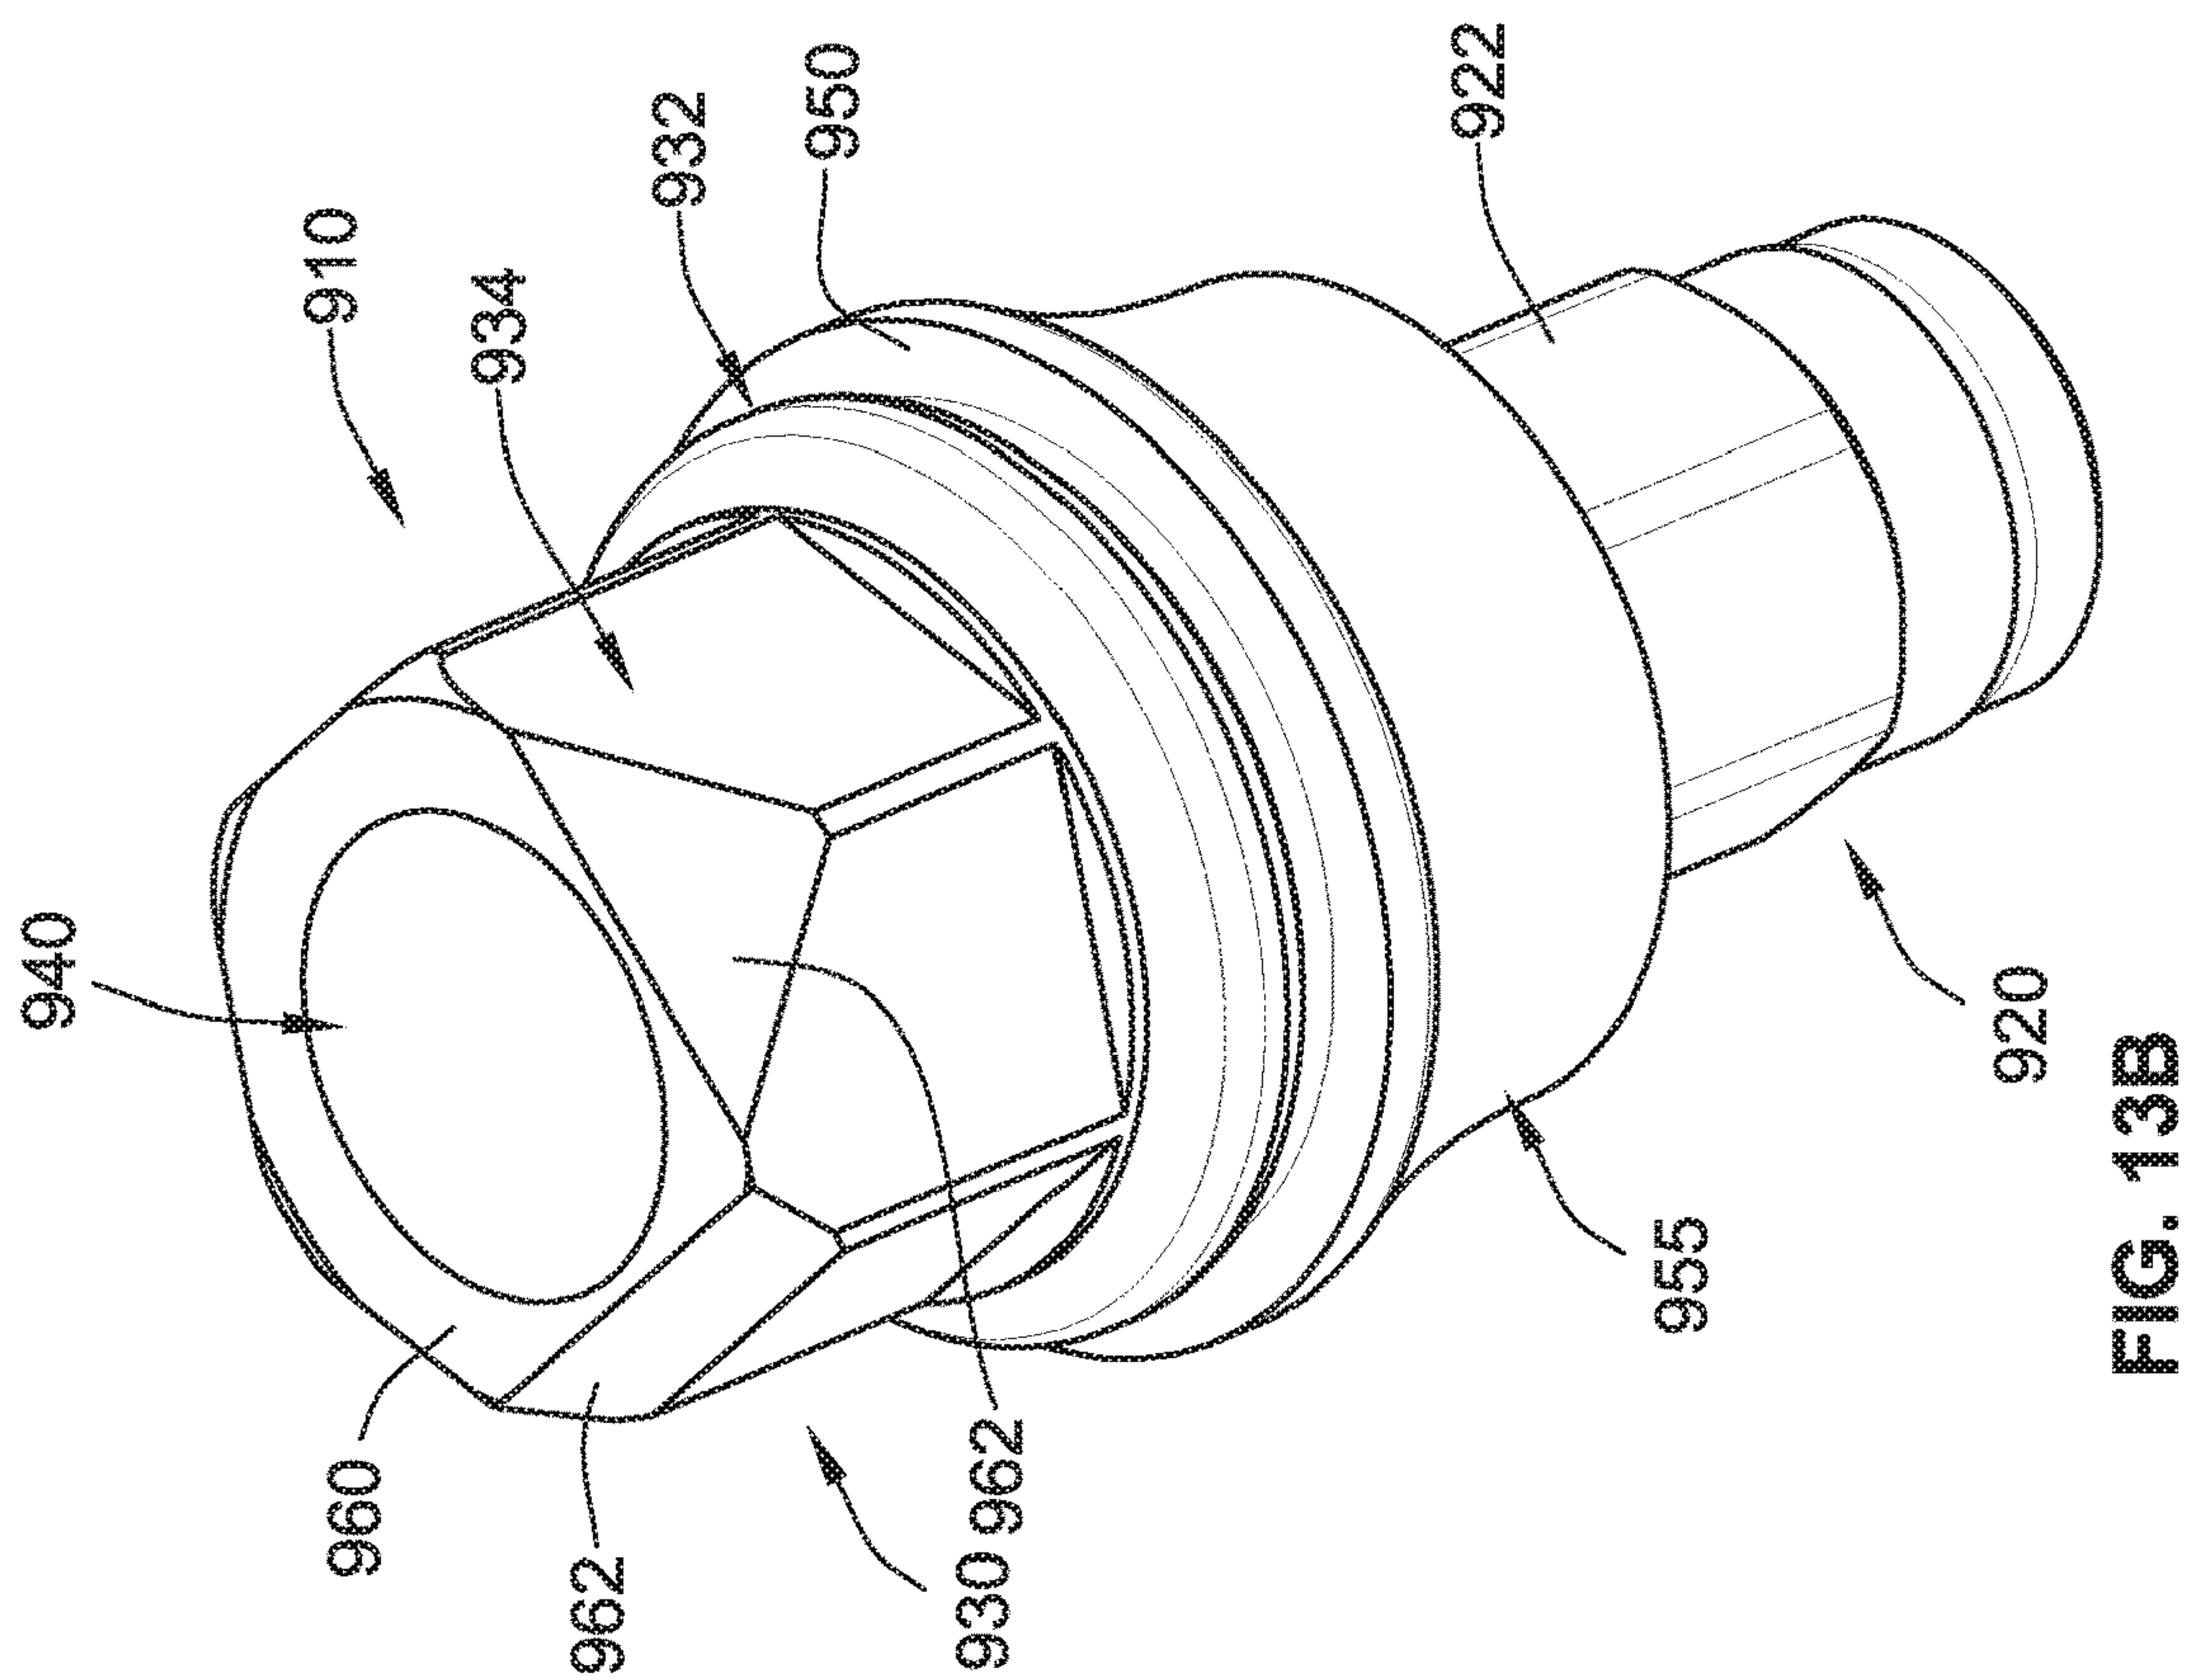
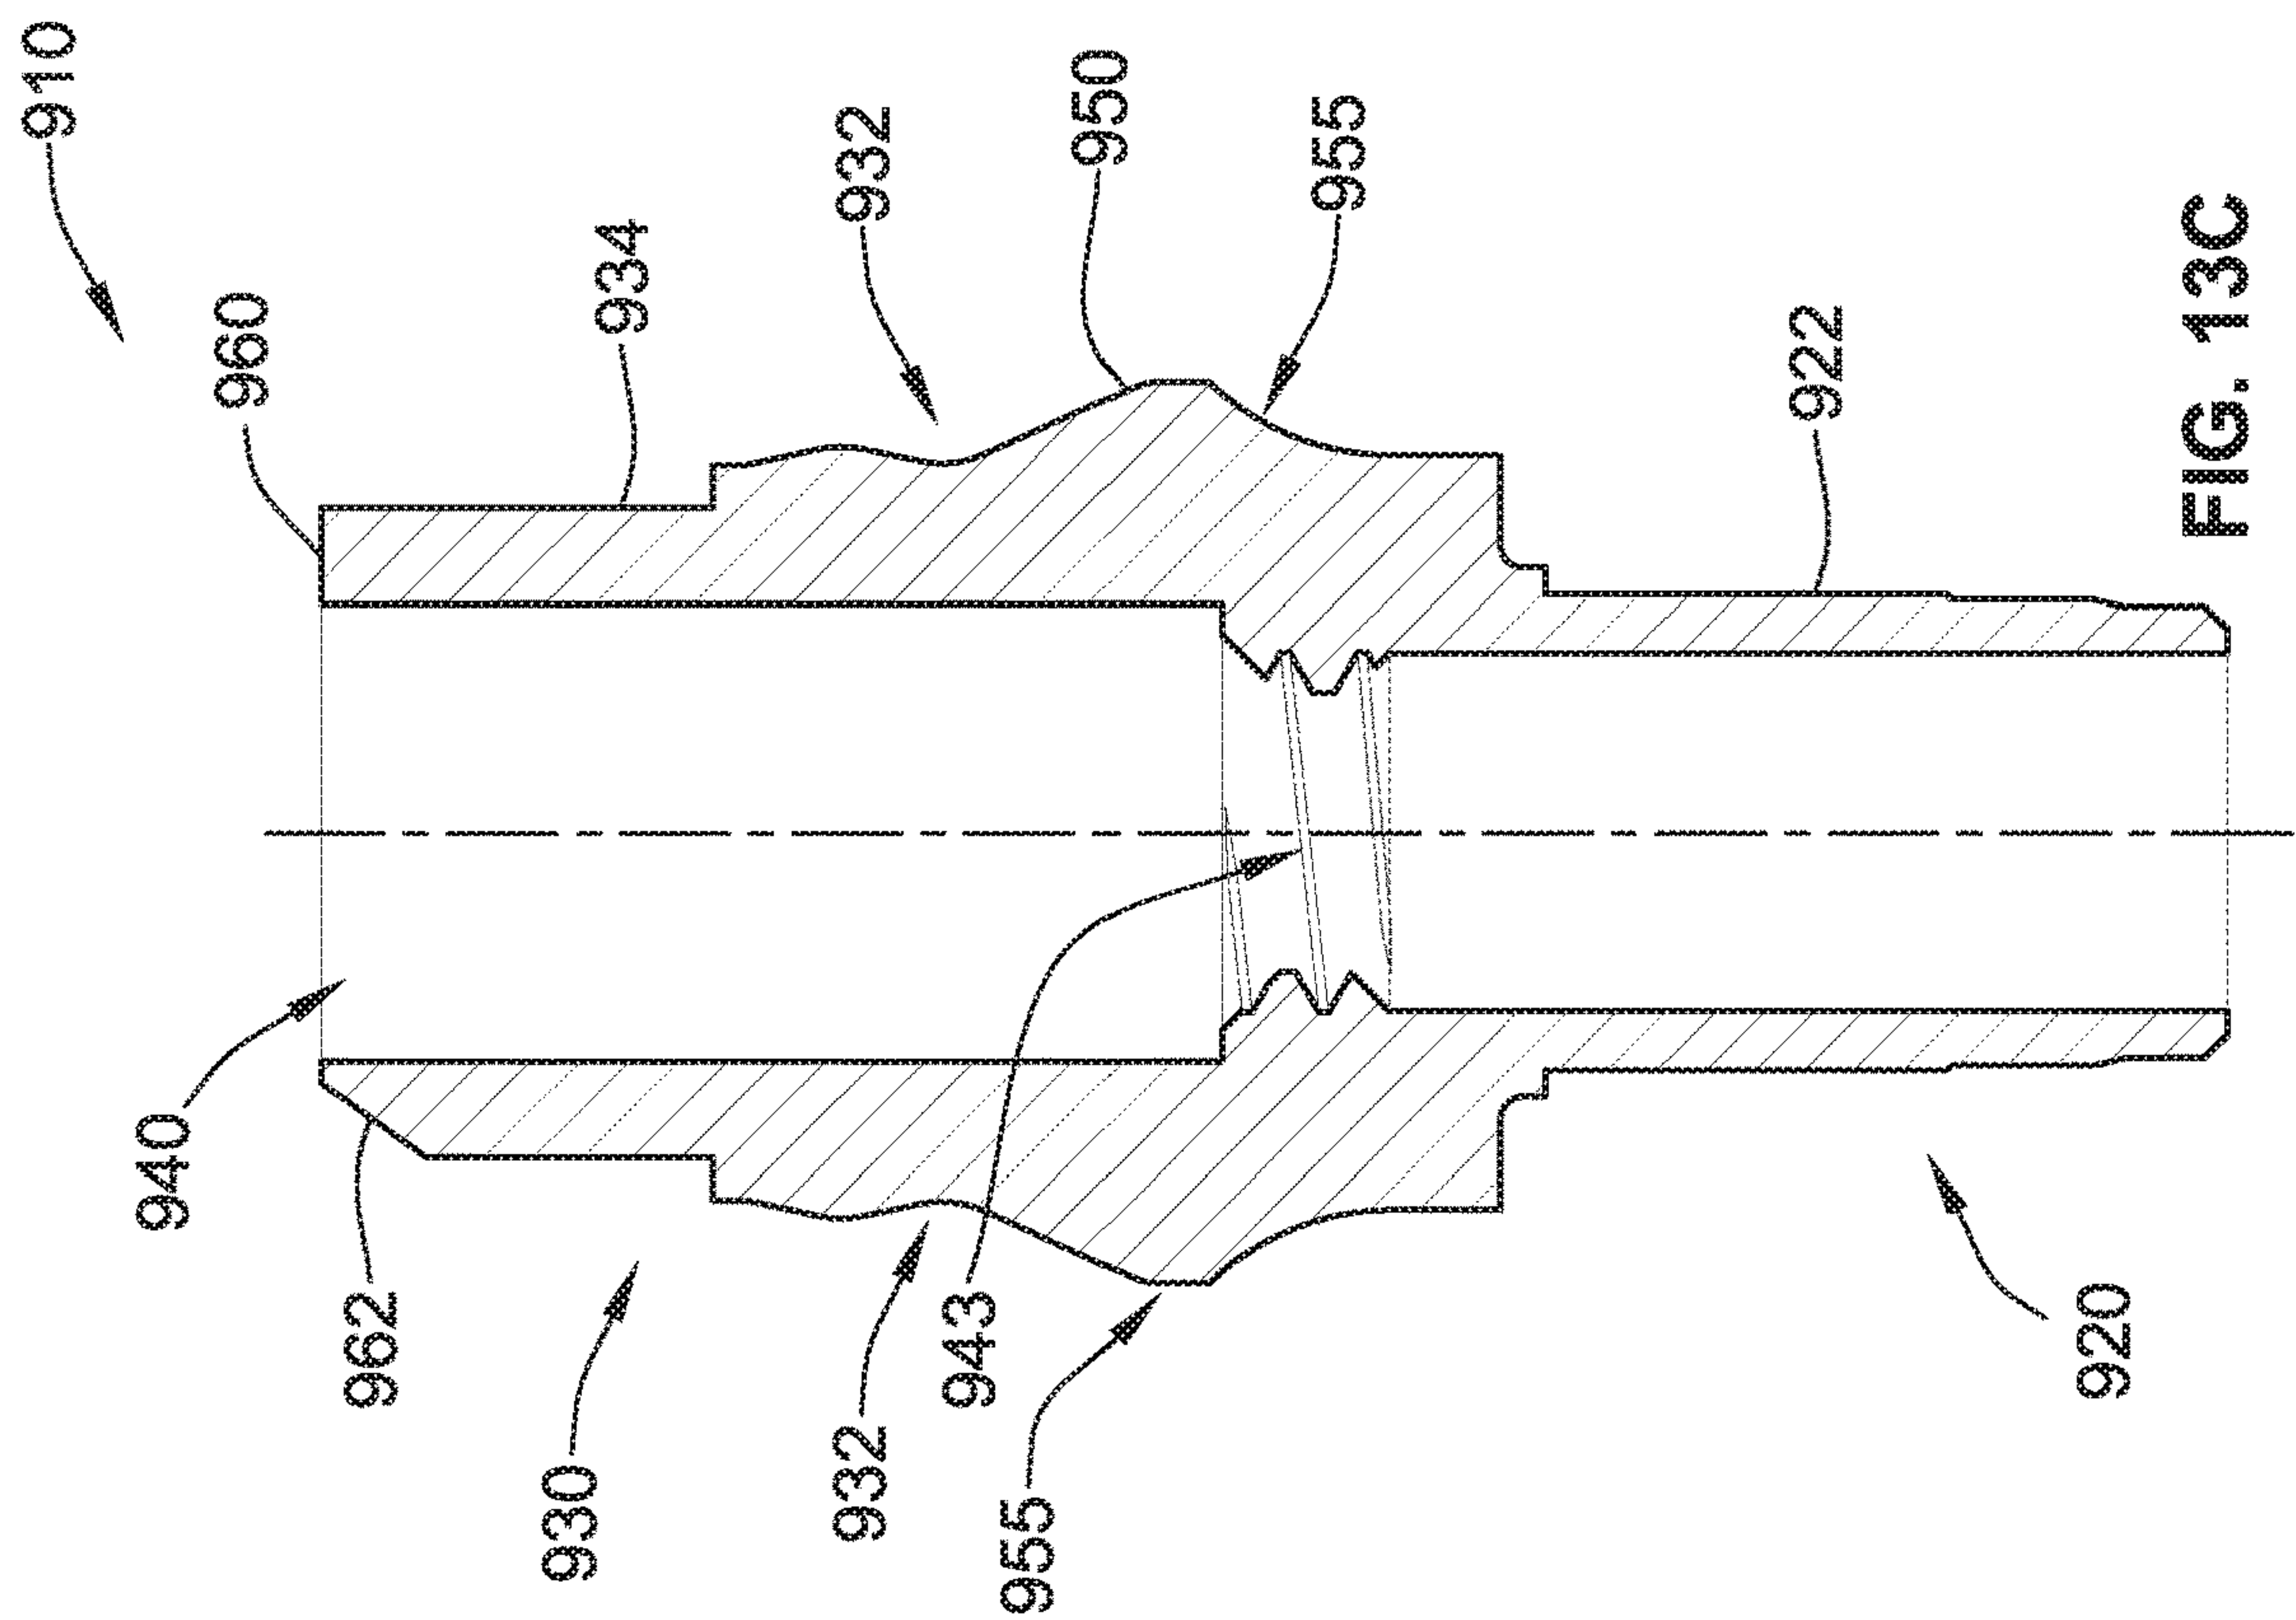
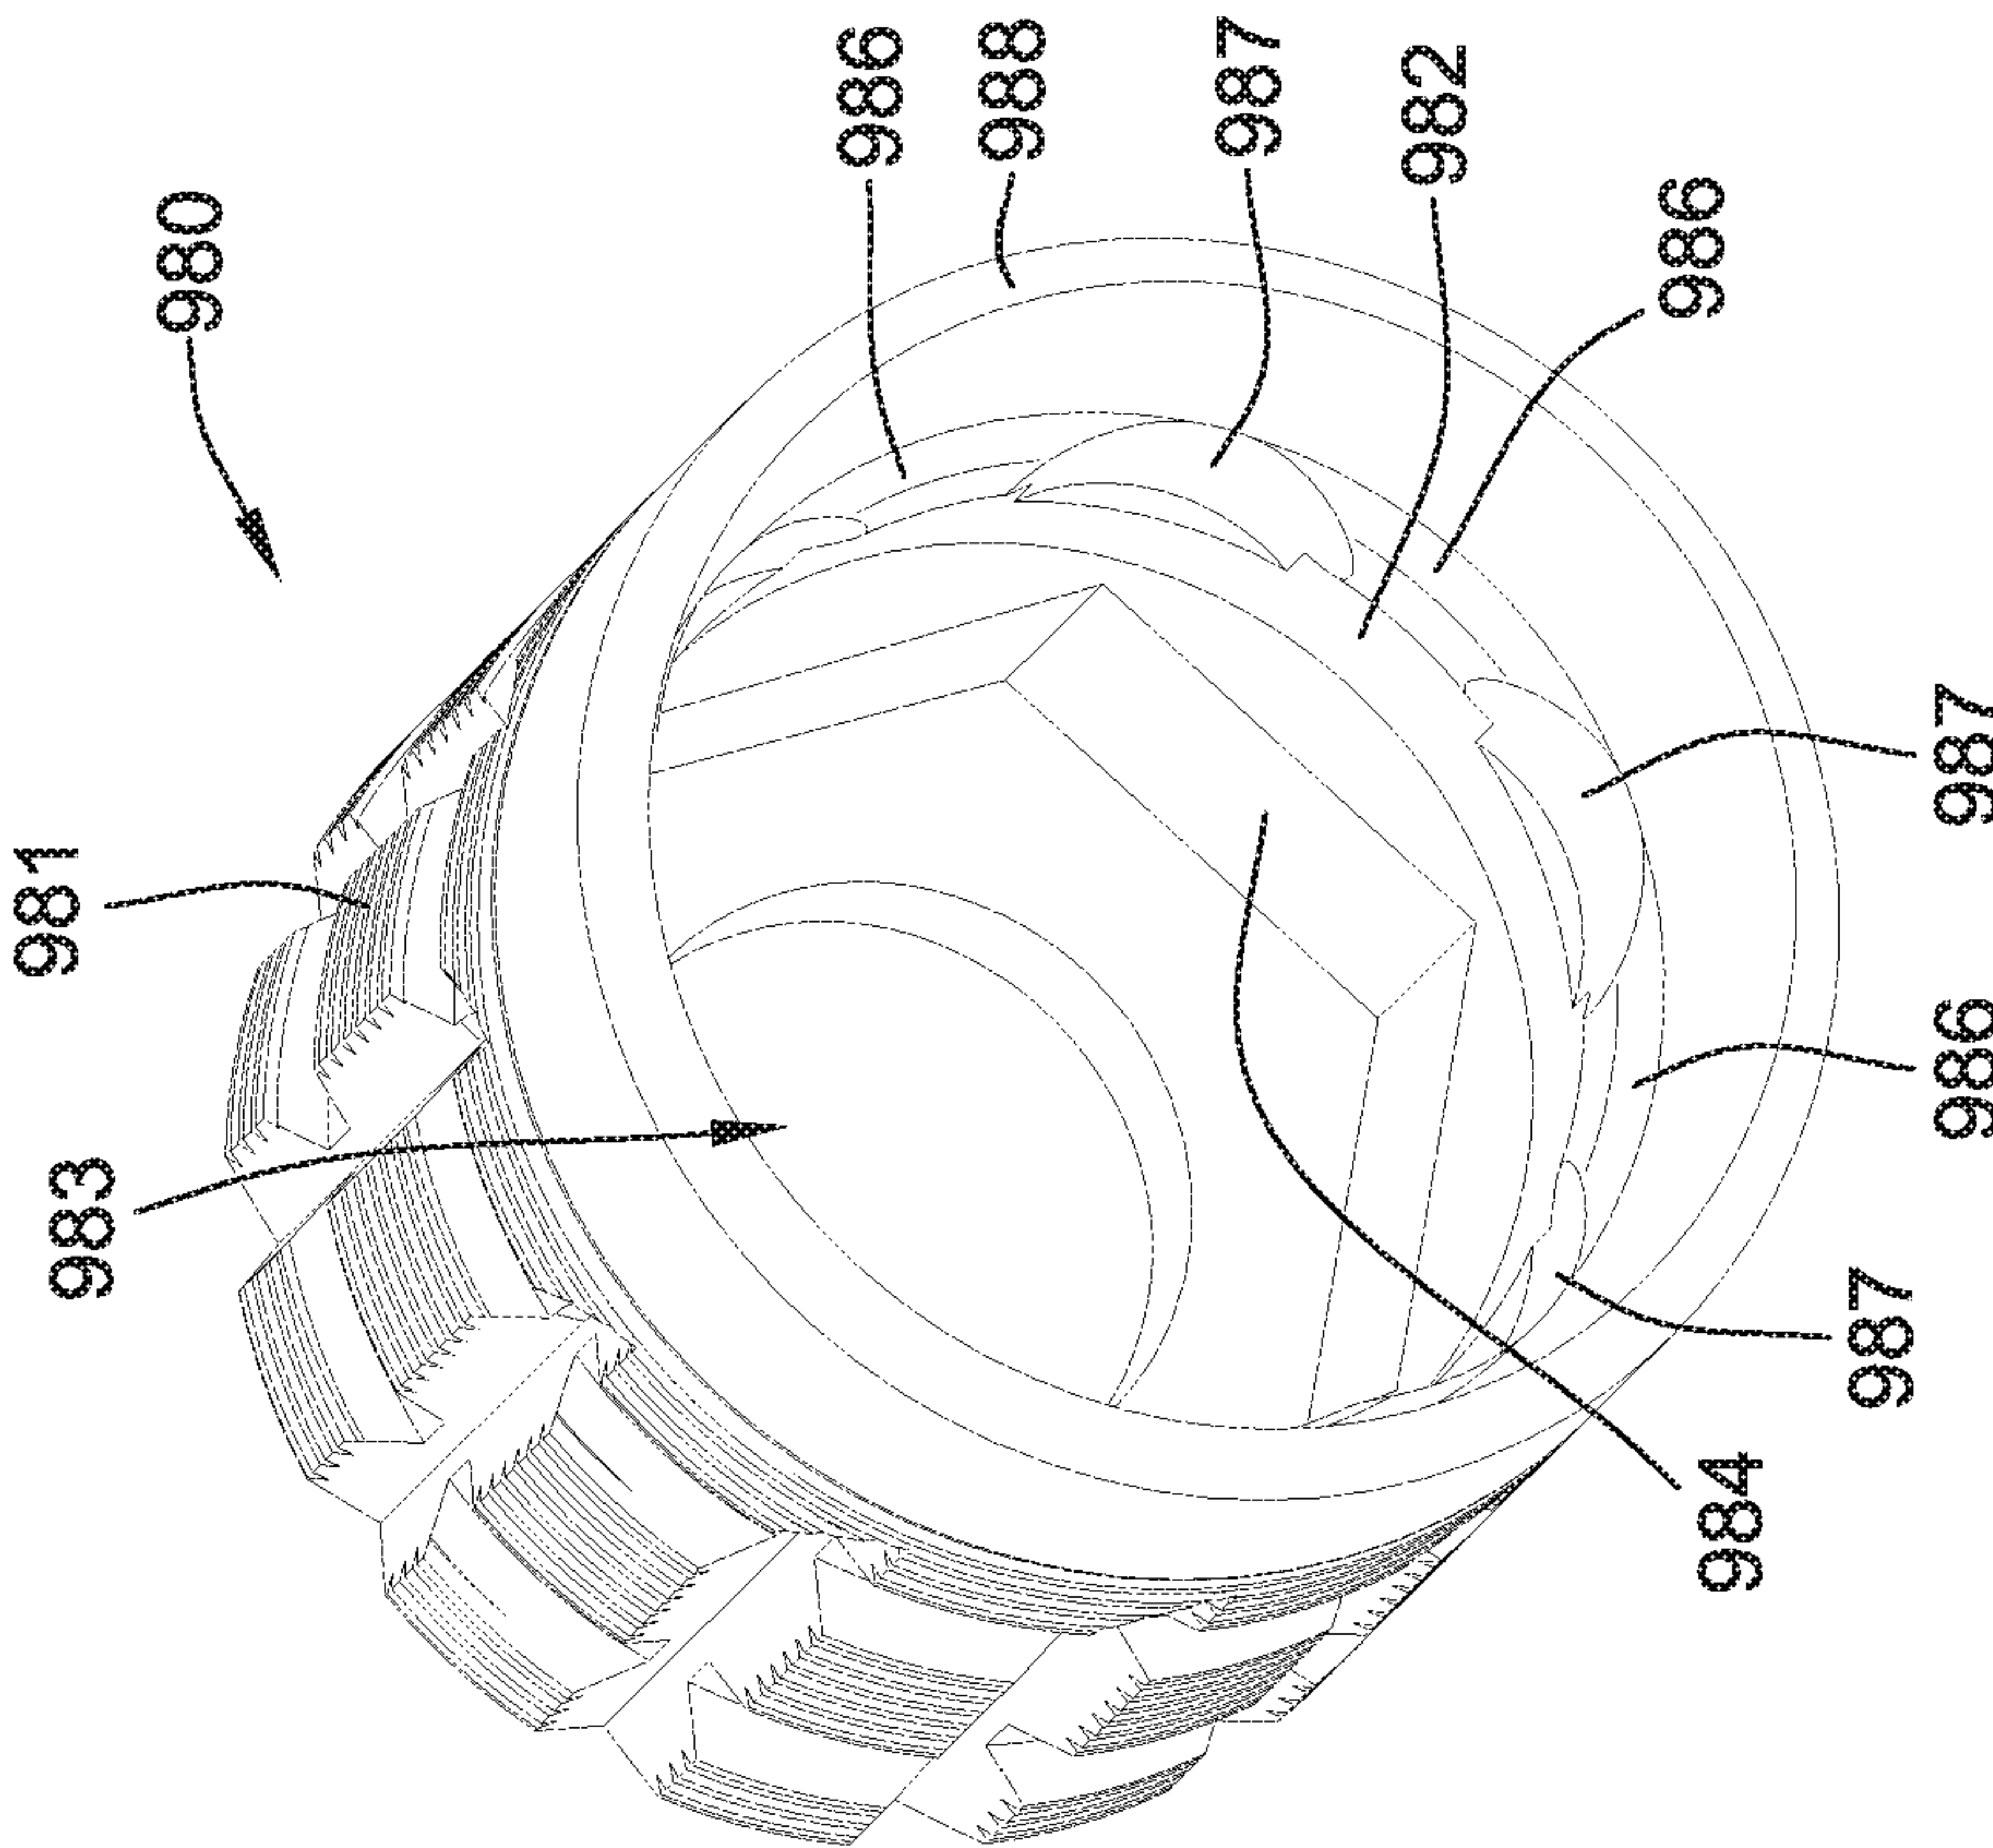
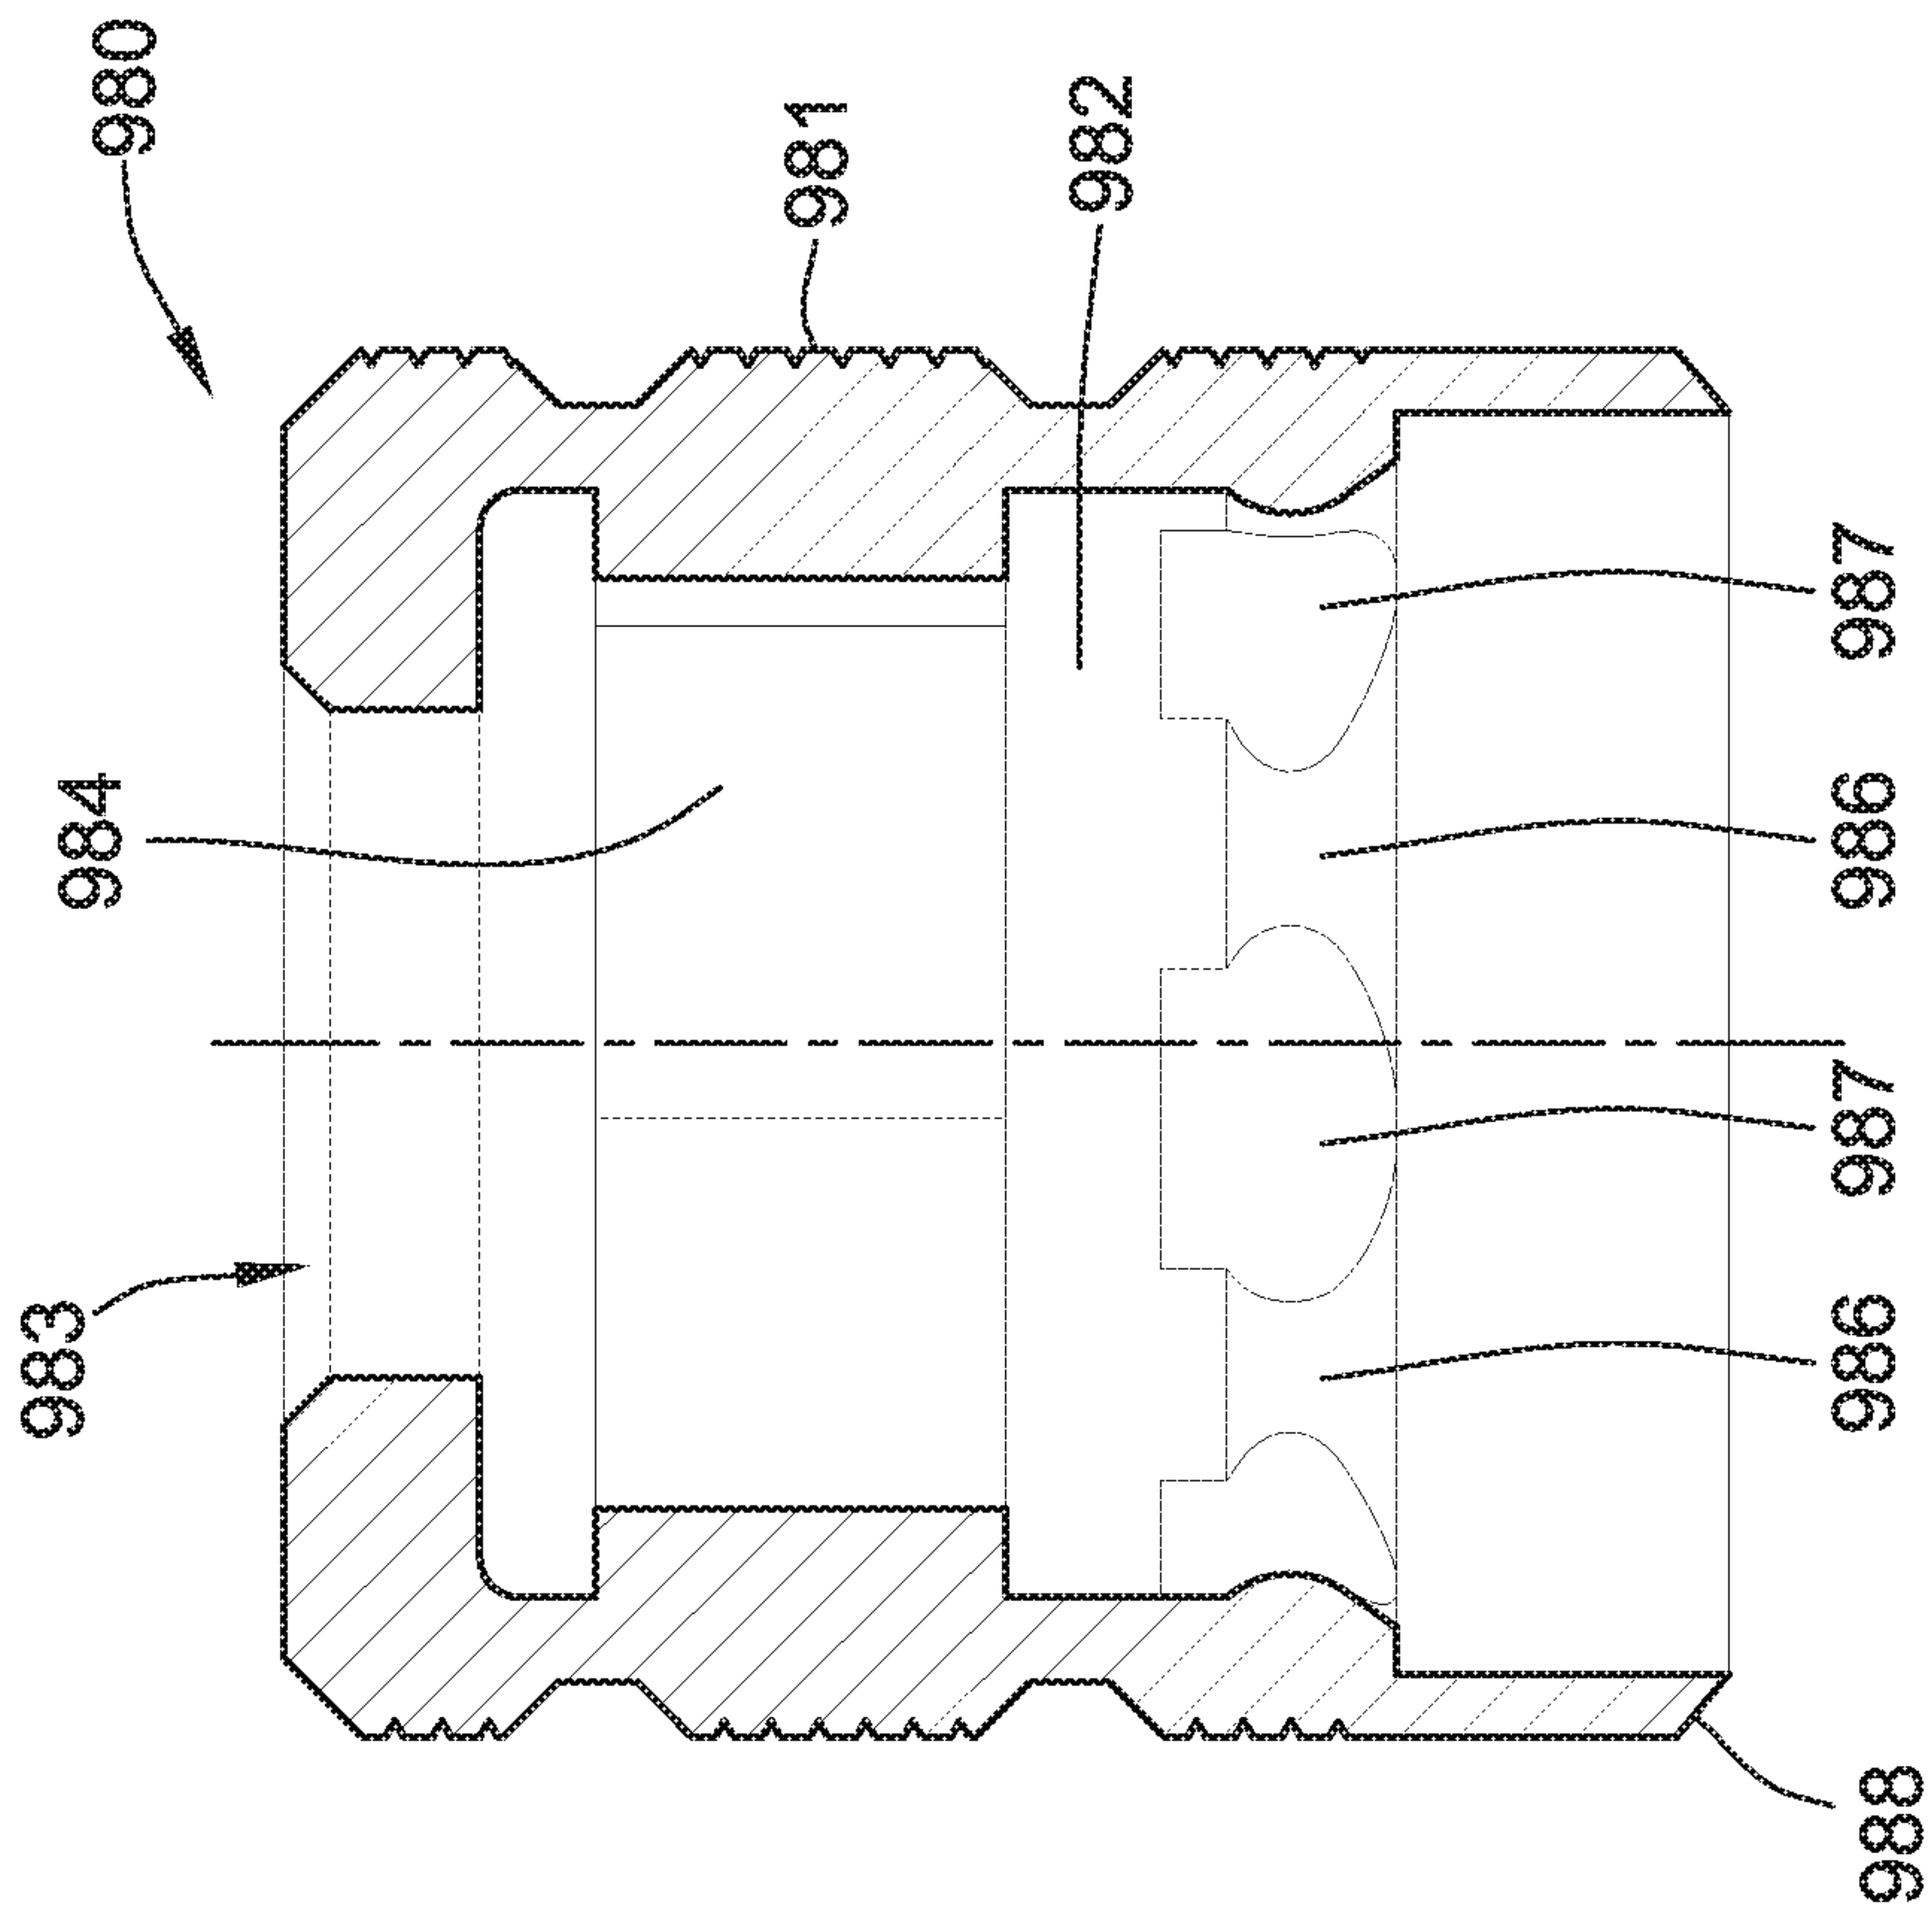


FIG. 13F









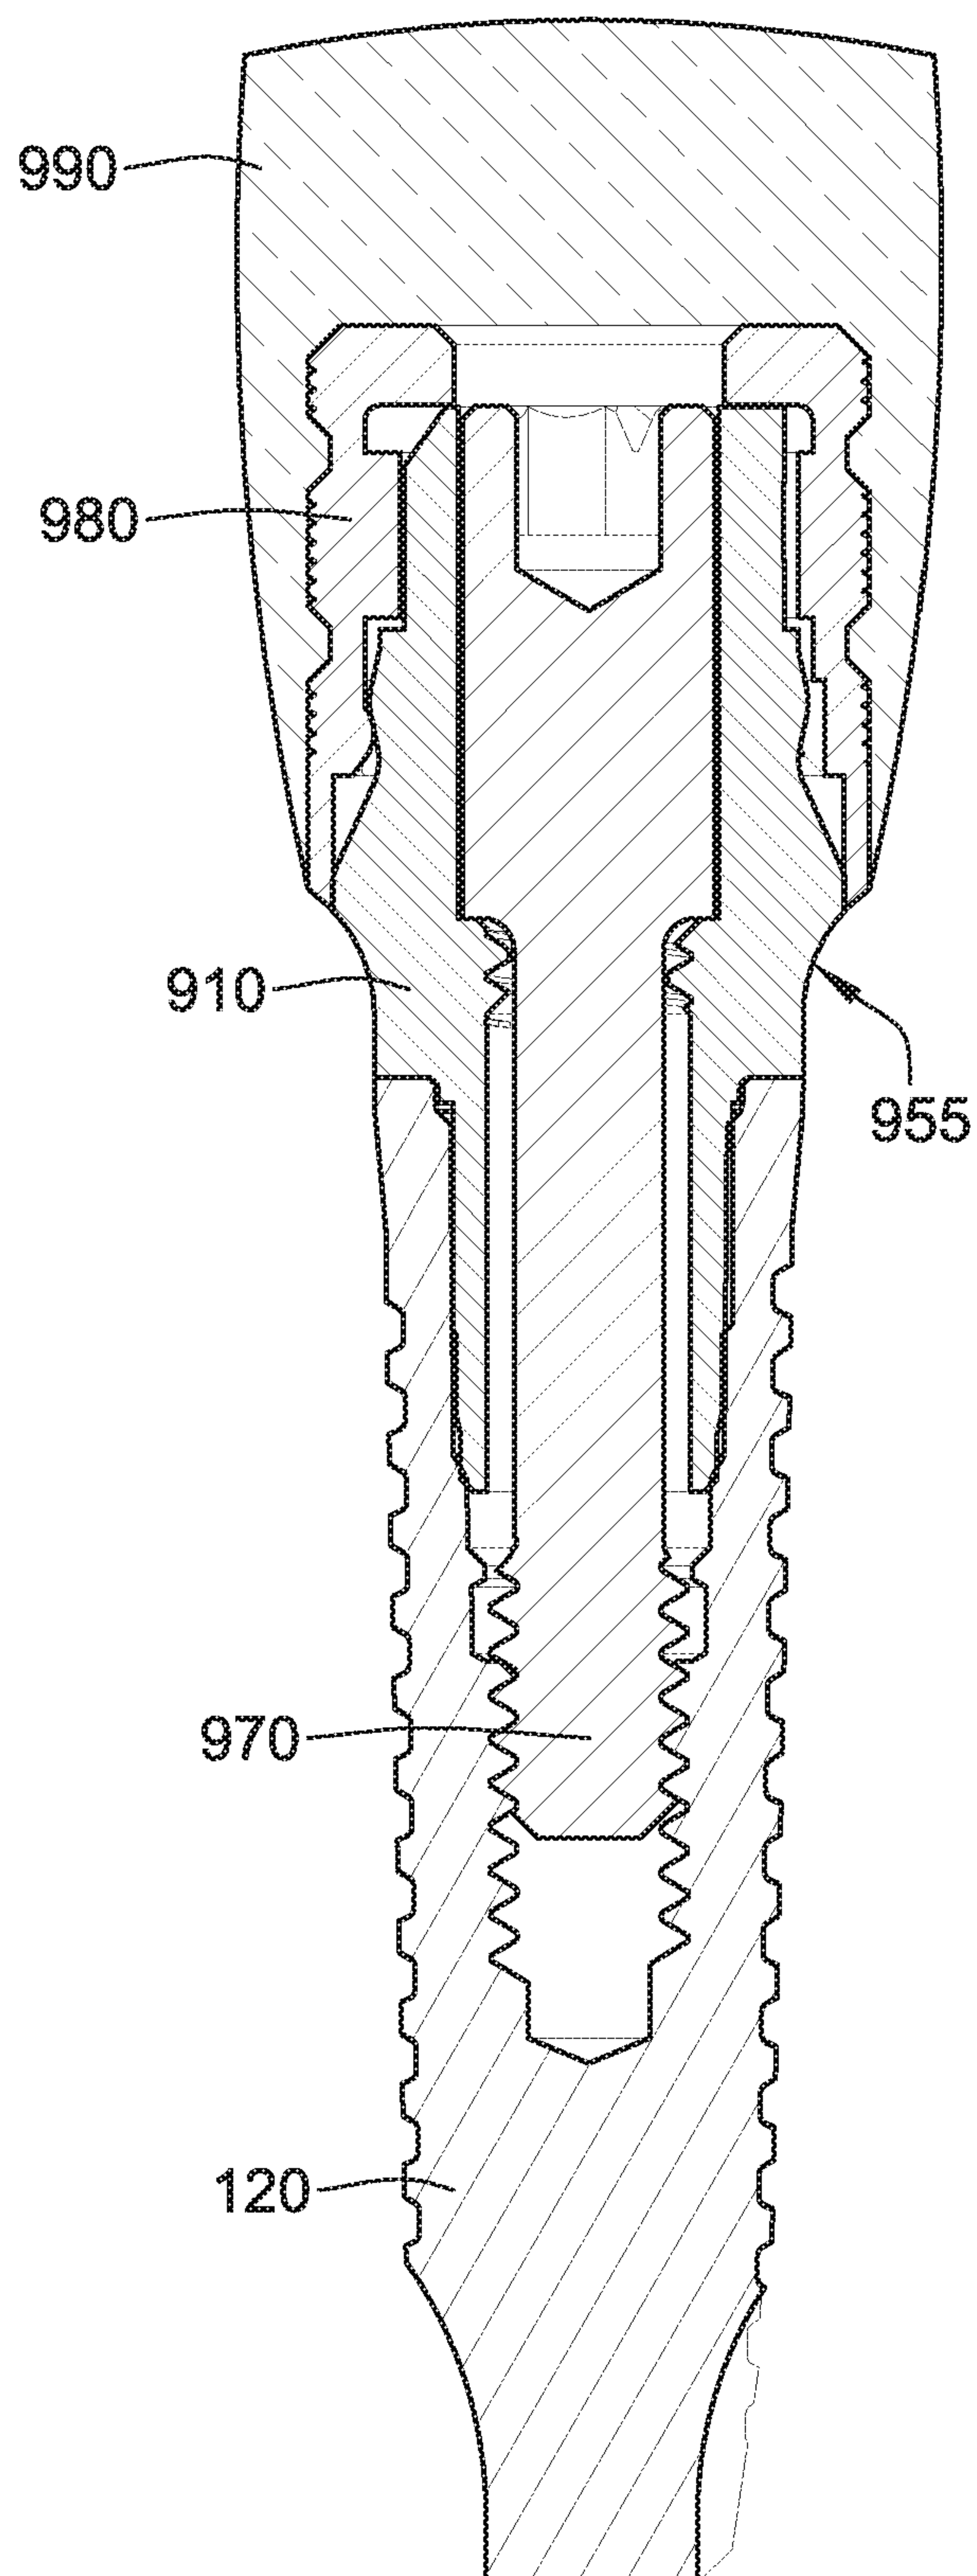


FIG. 13G

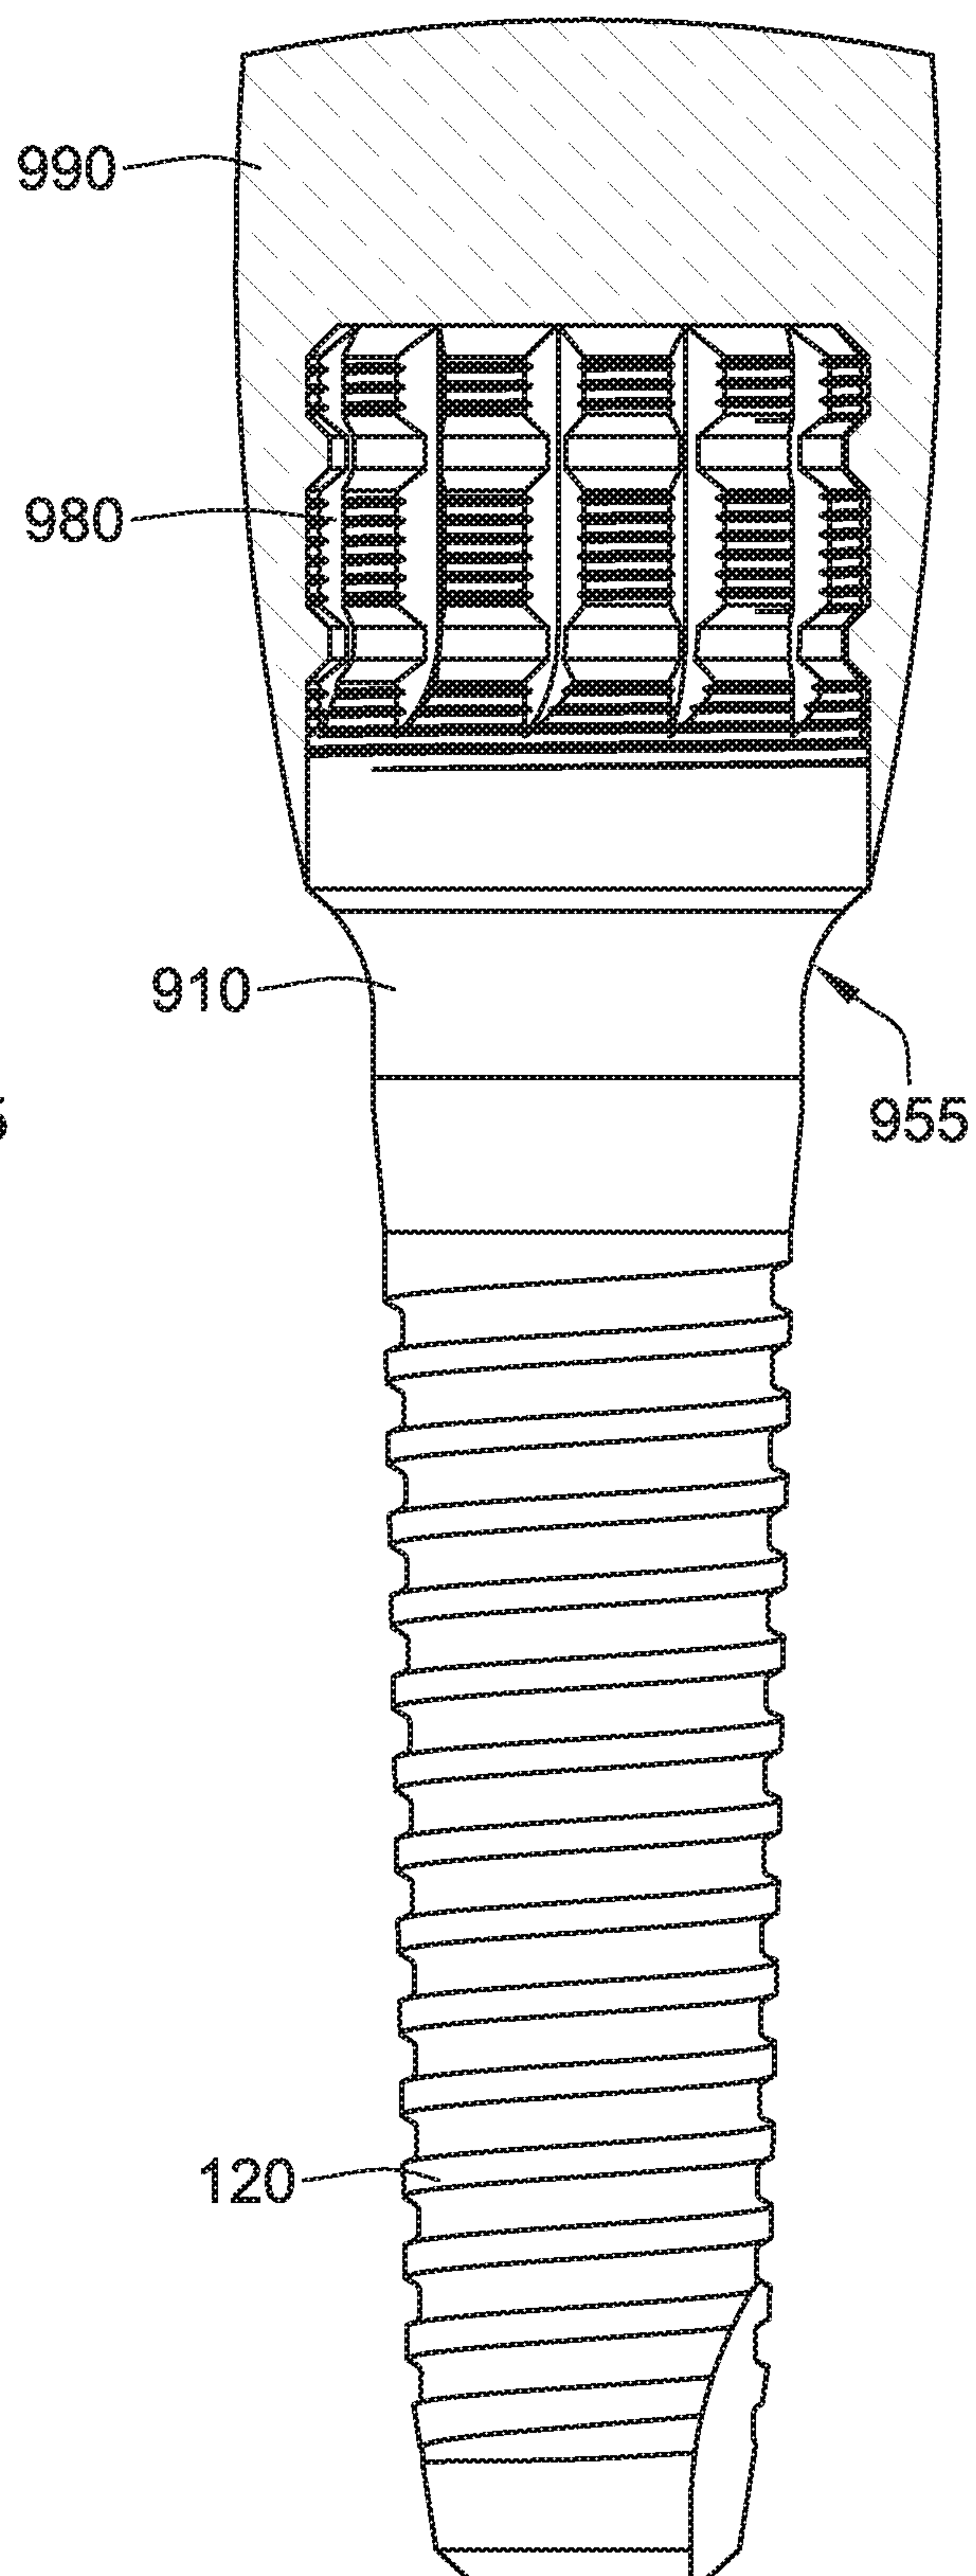


FIG. 13H

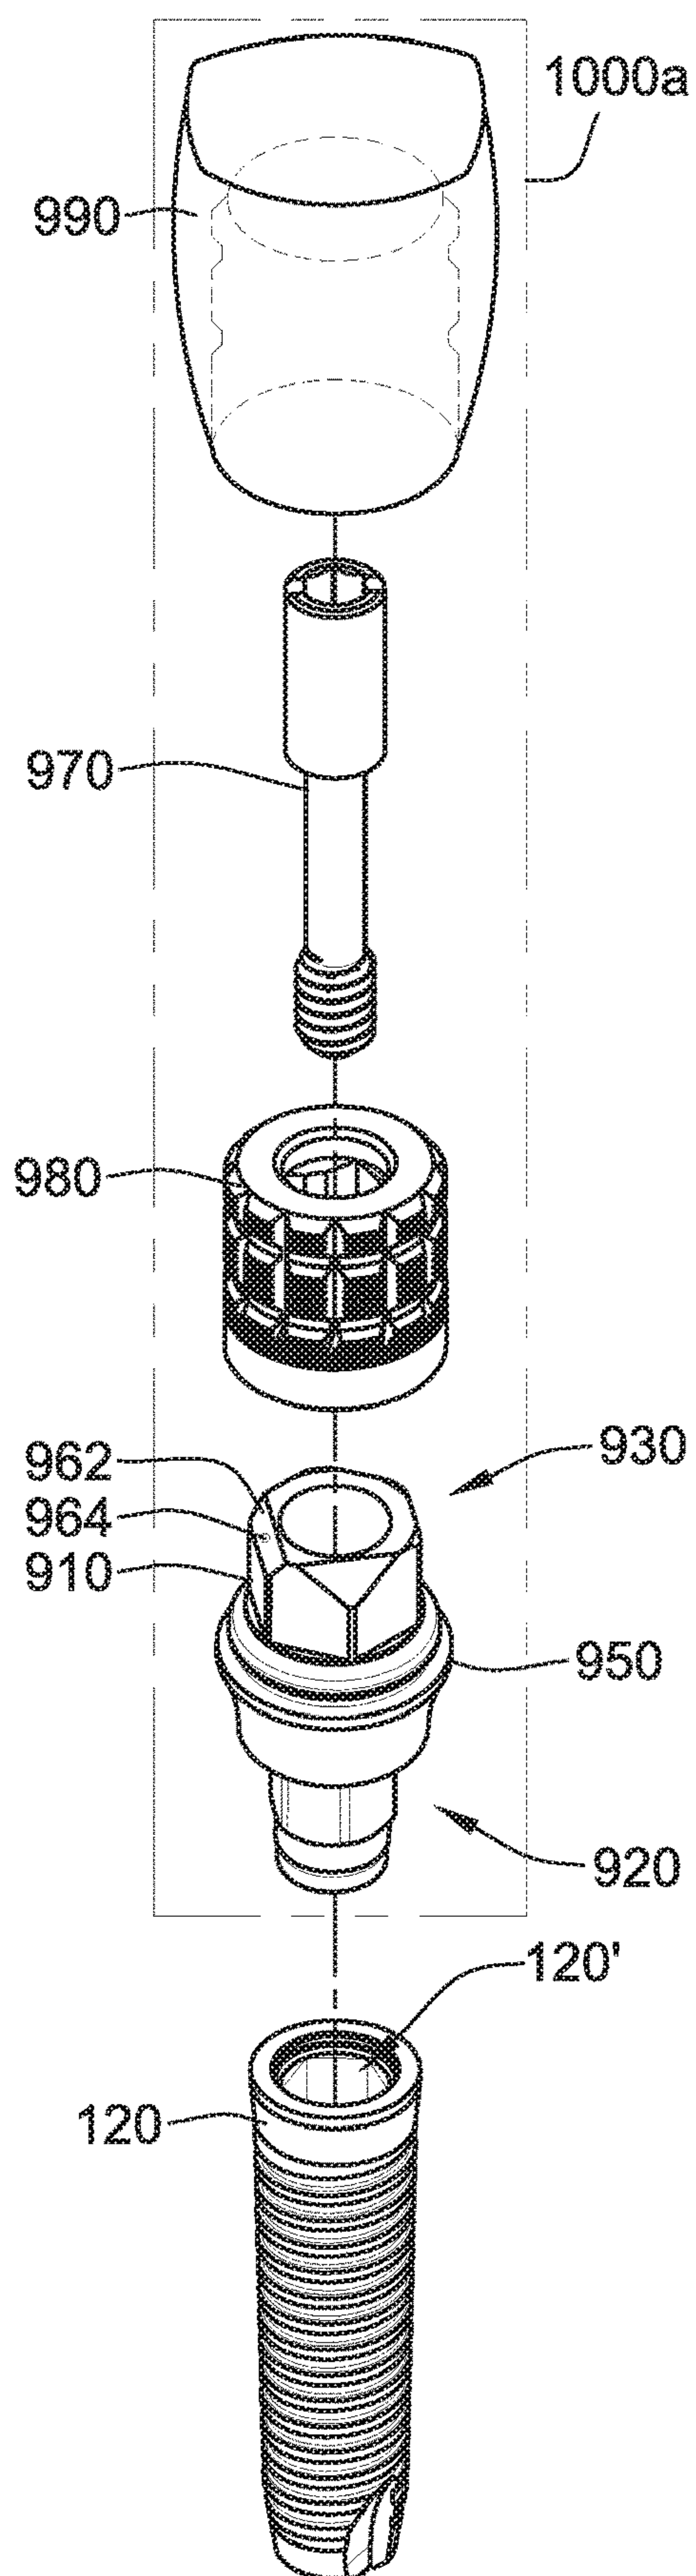


FIG. 14A

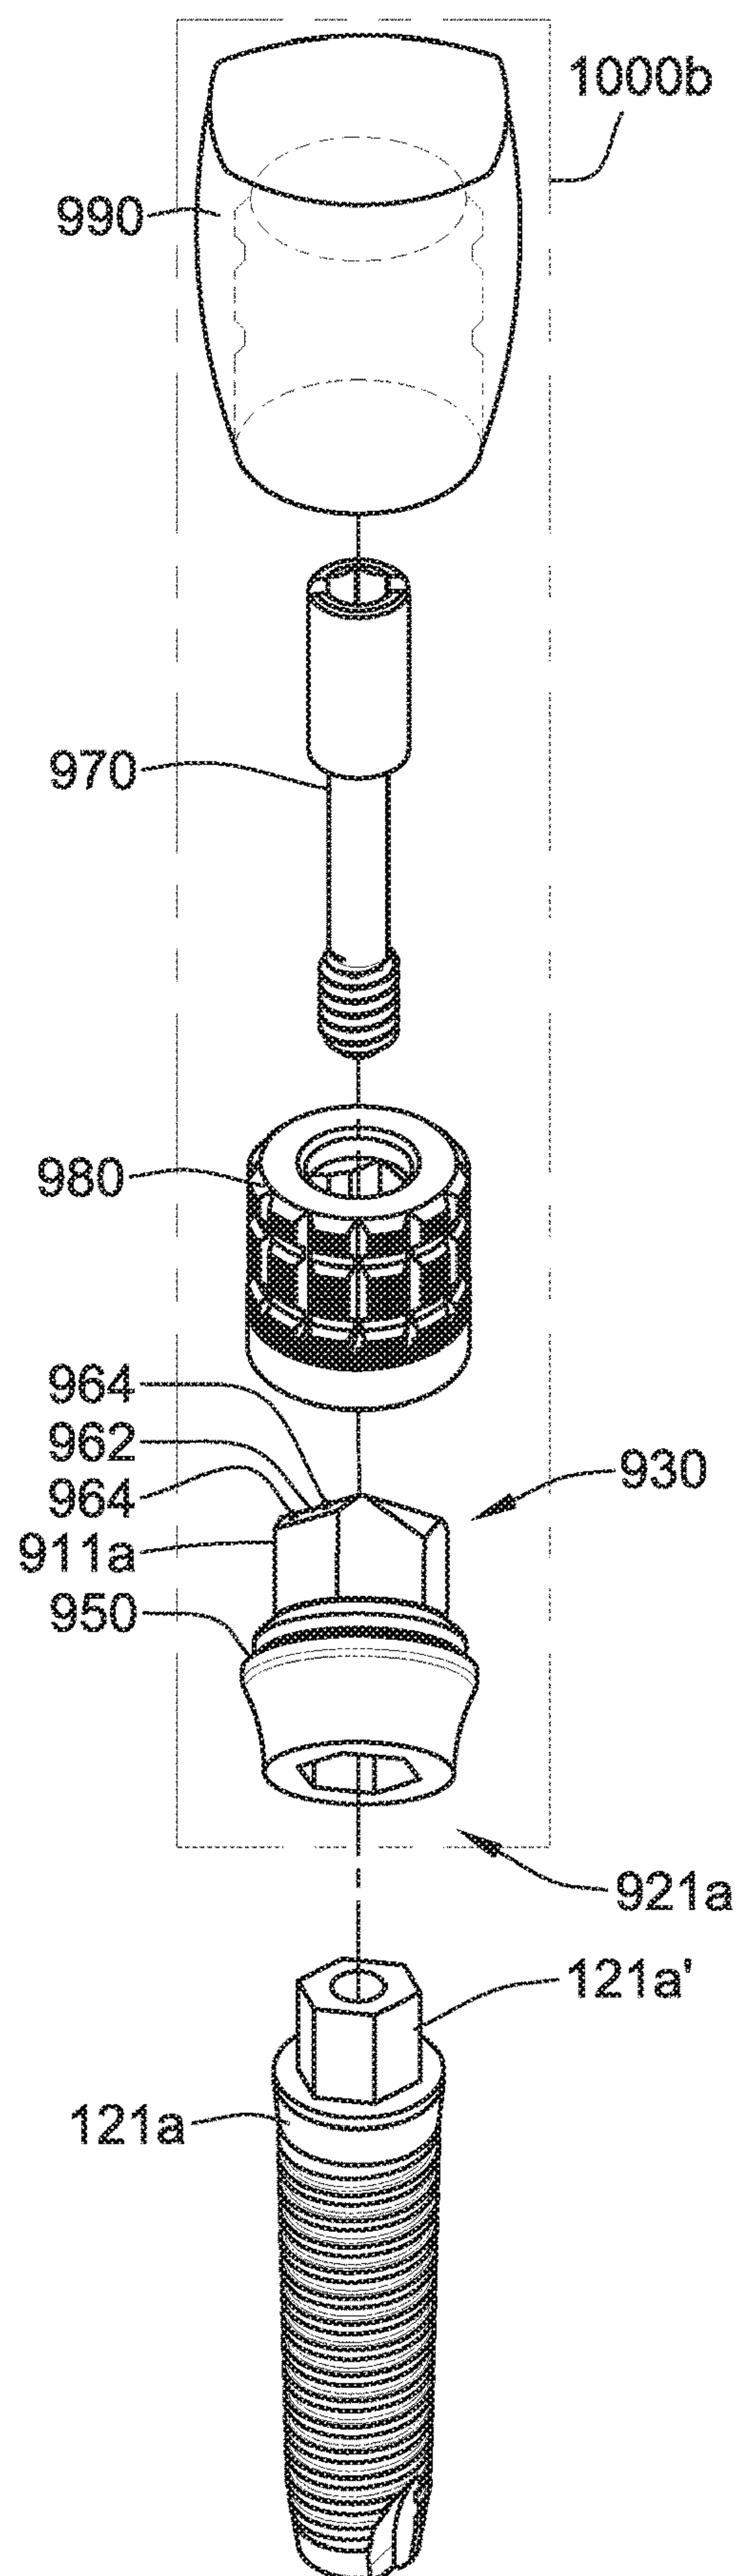


FIG. 14B



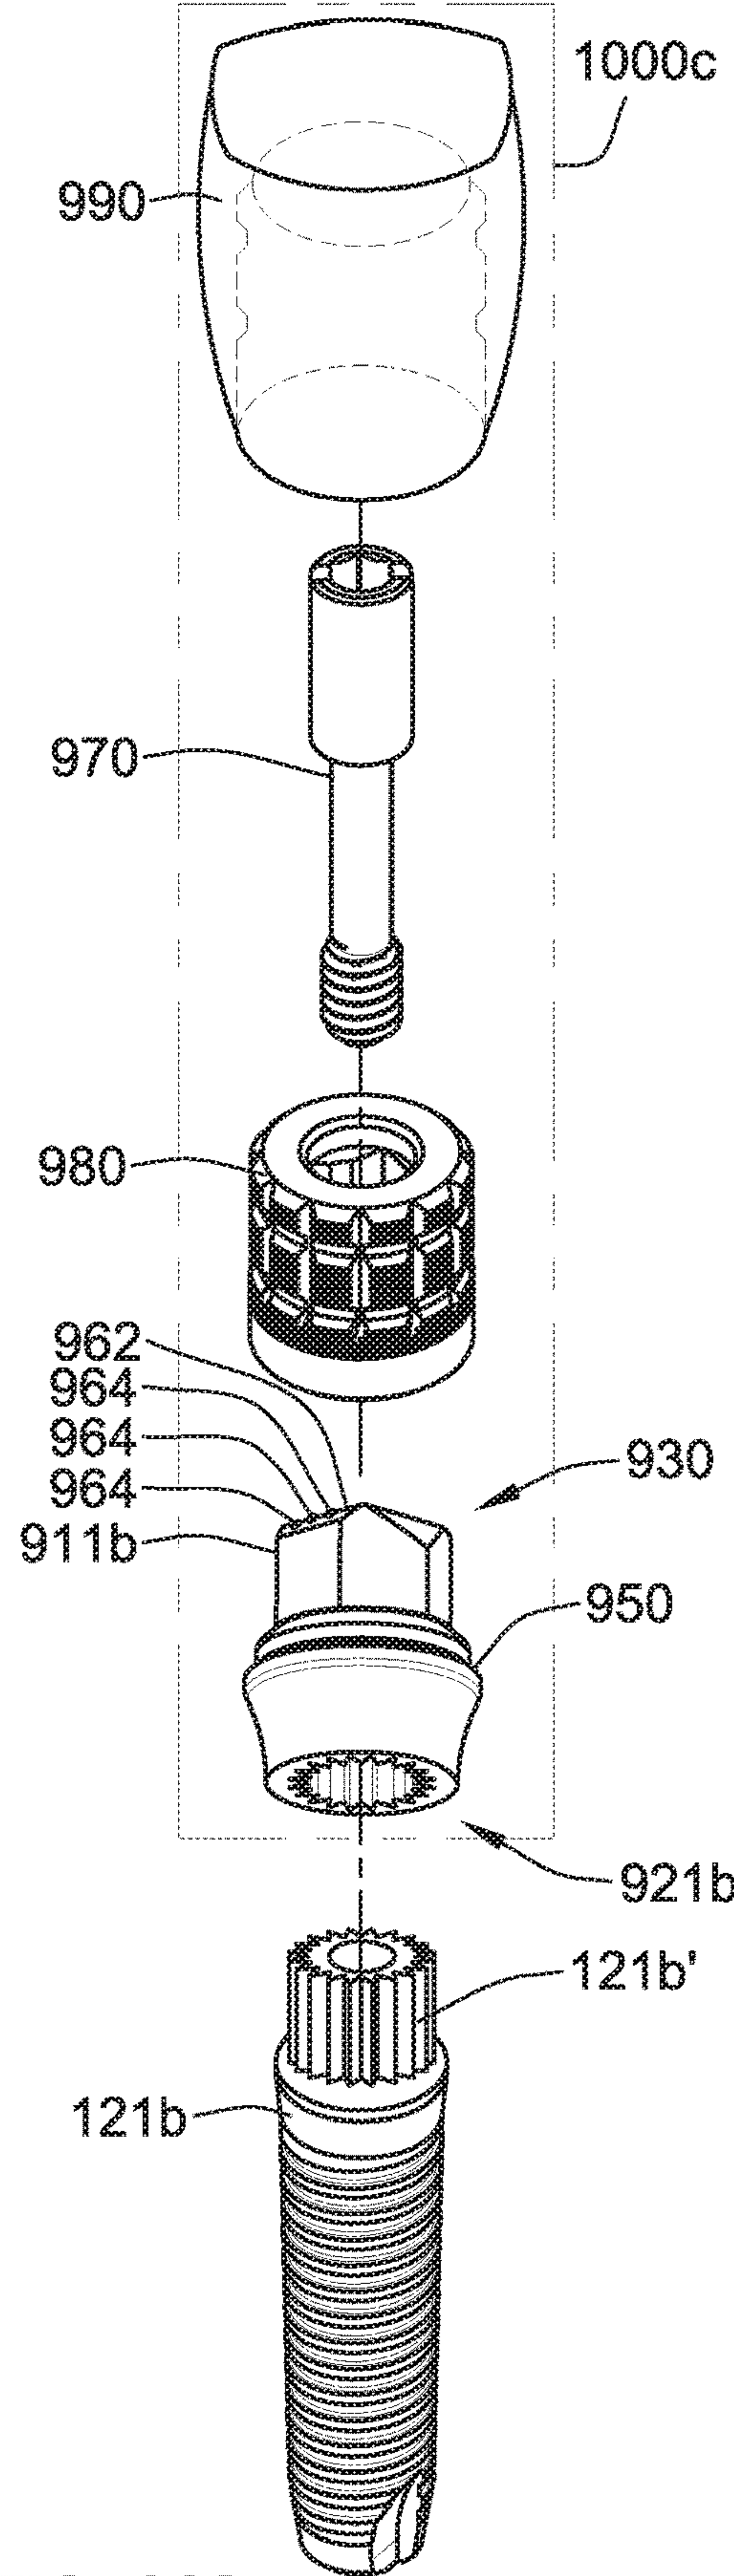


FIG. 14C

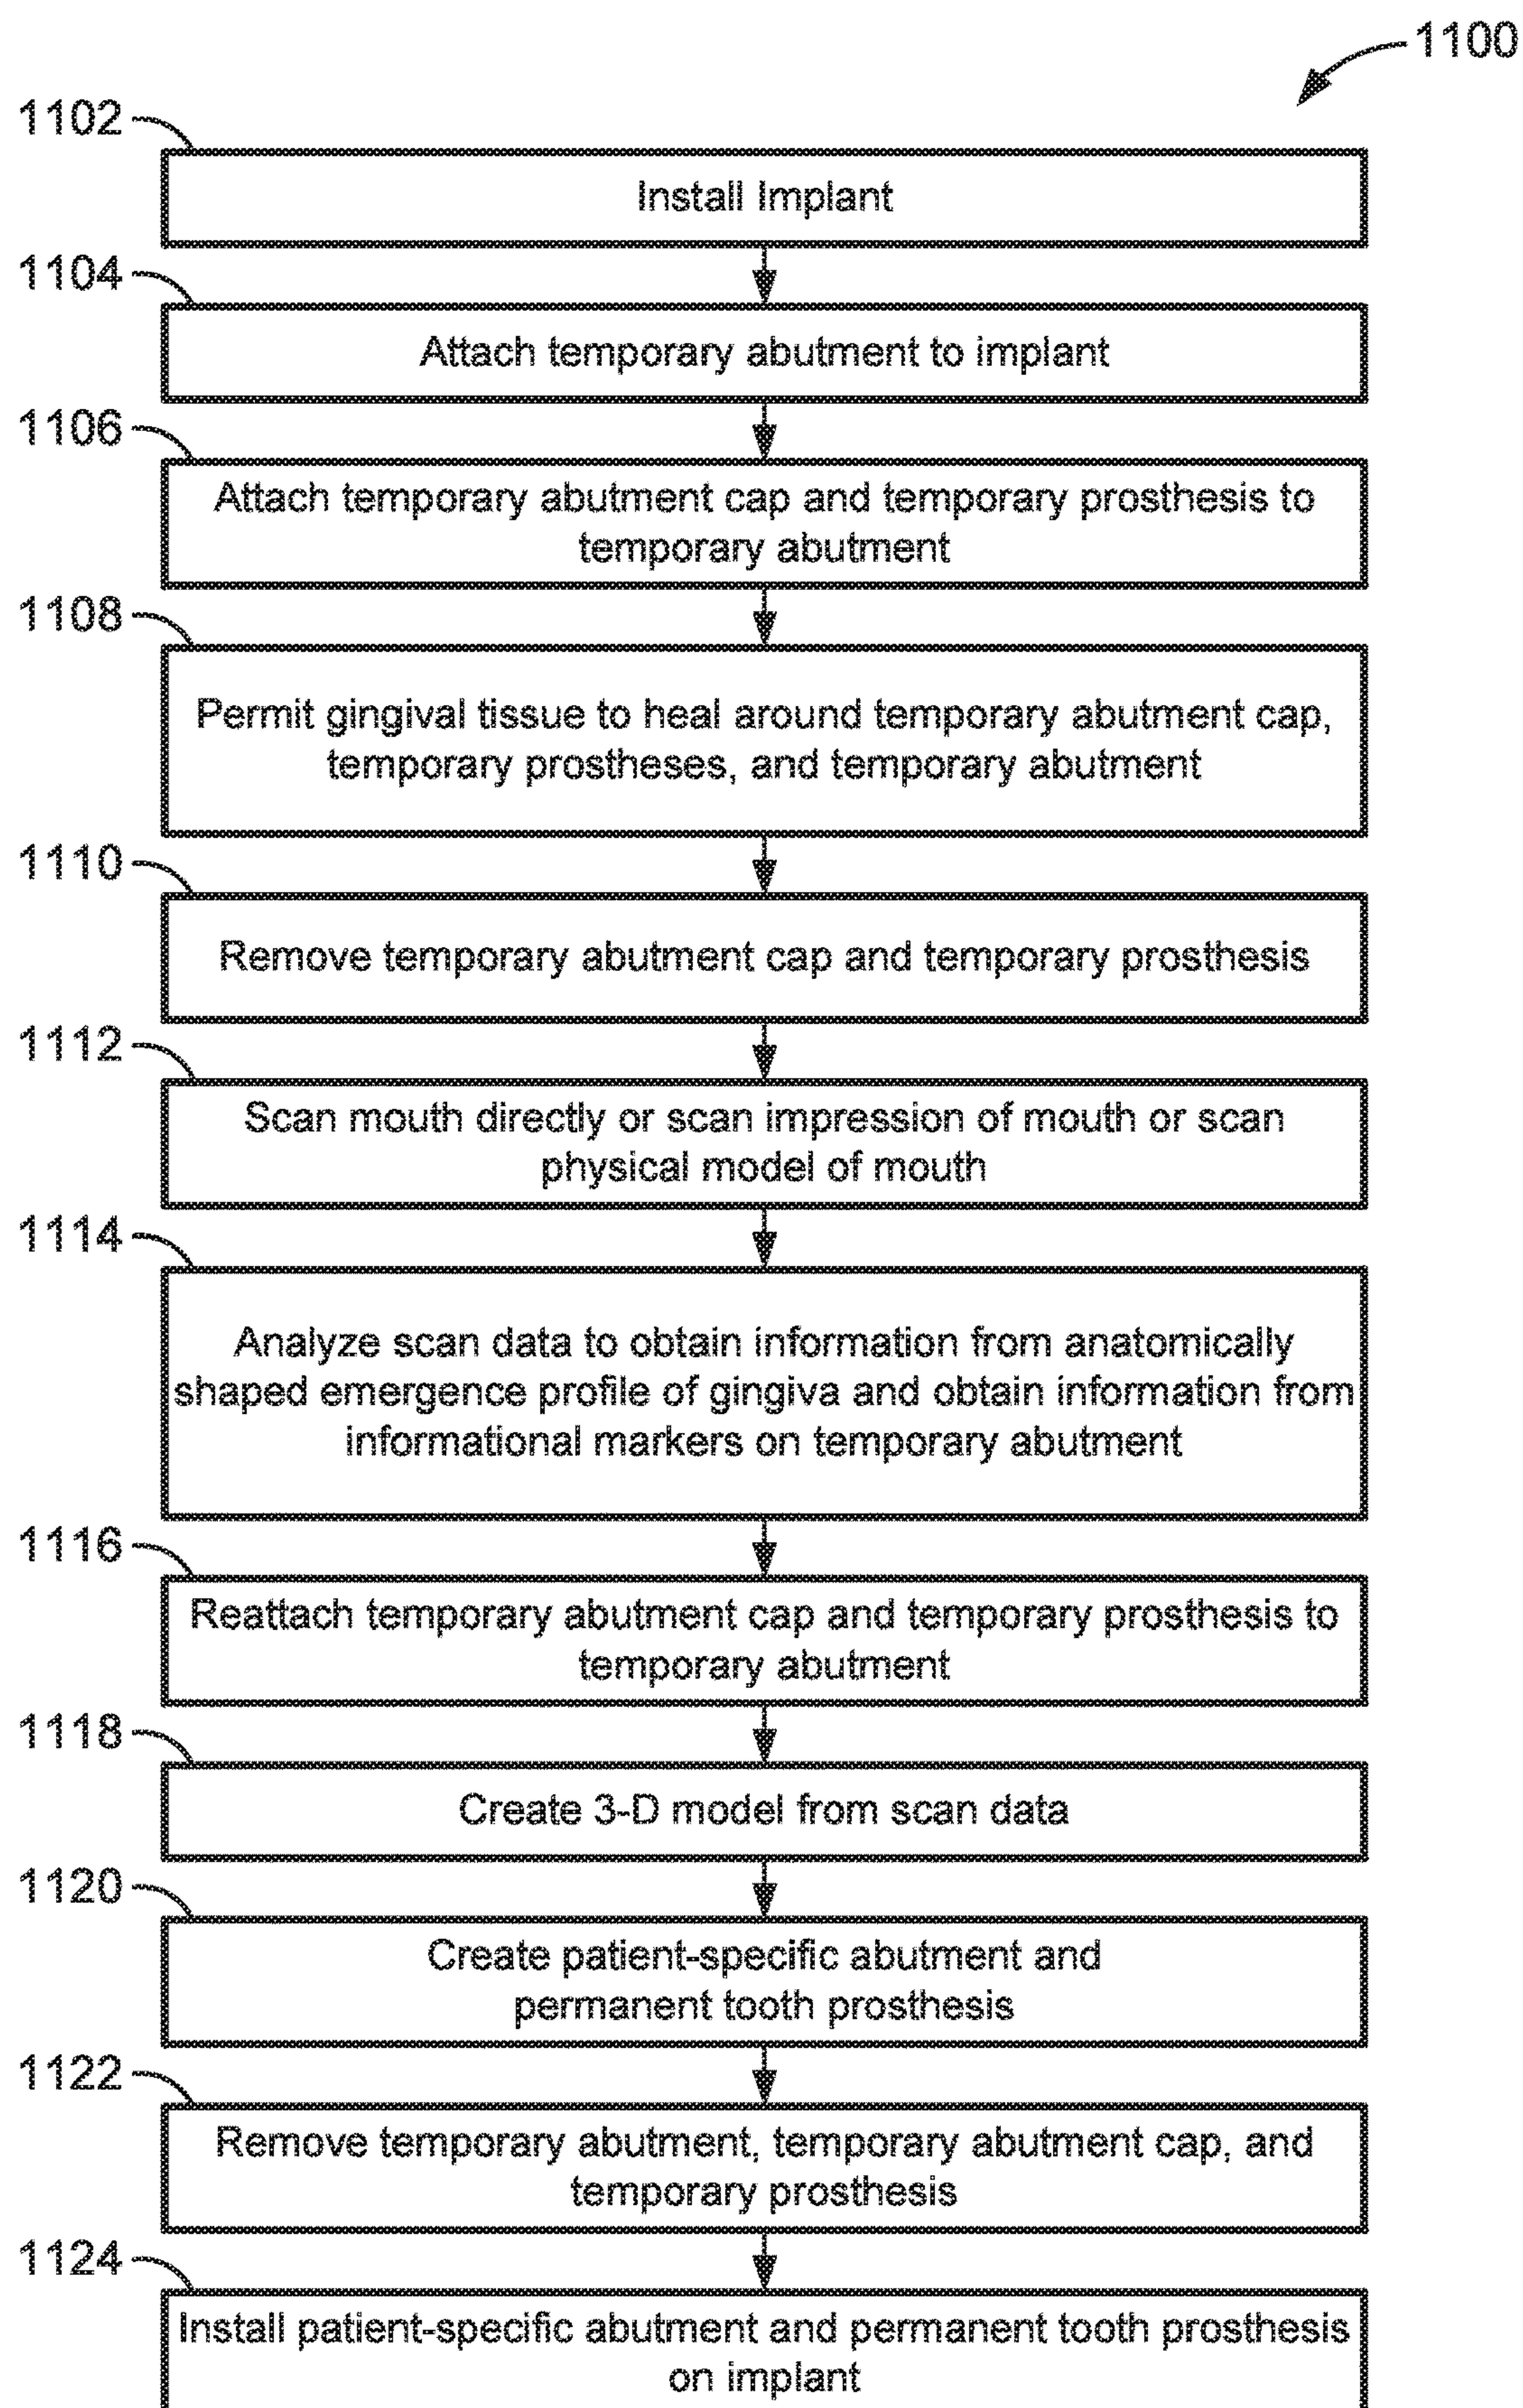


FIG. 15



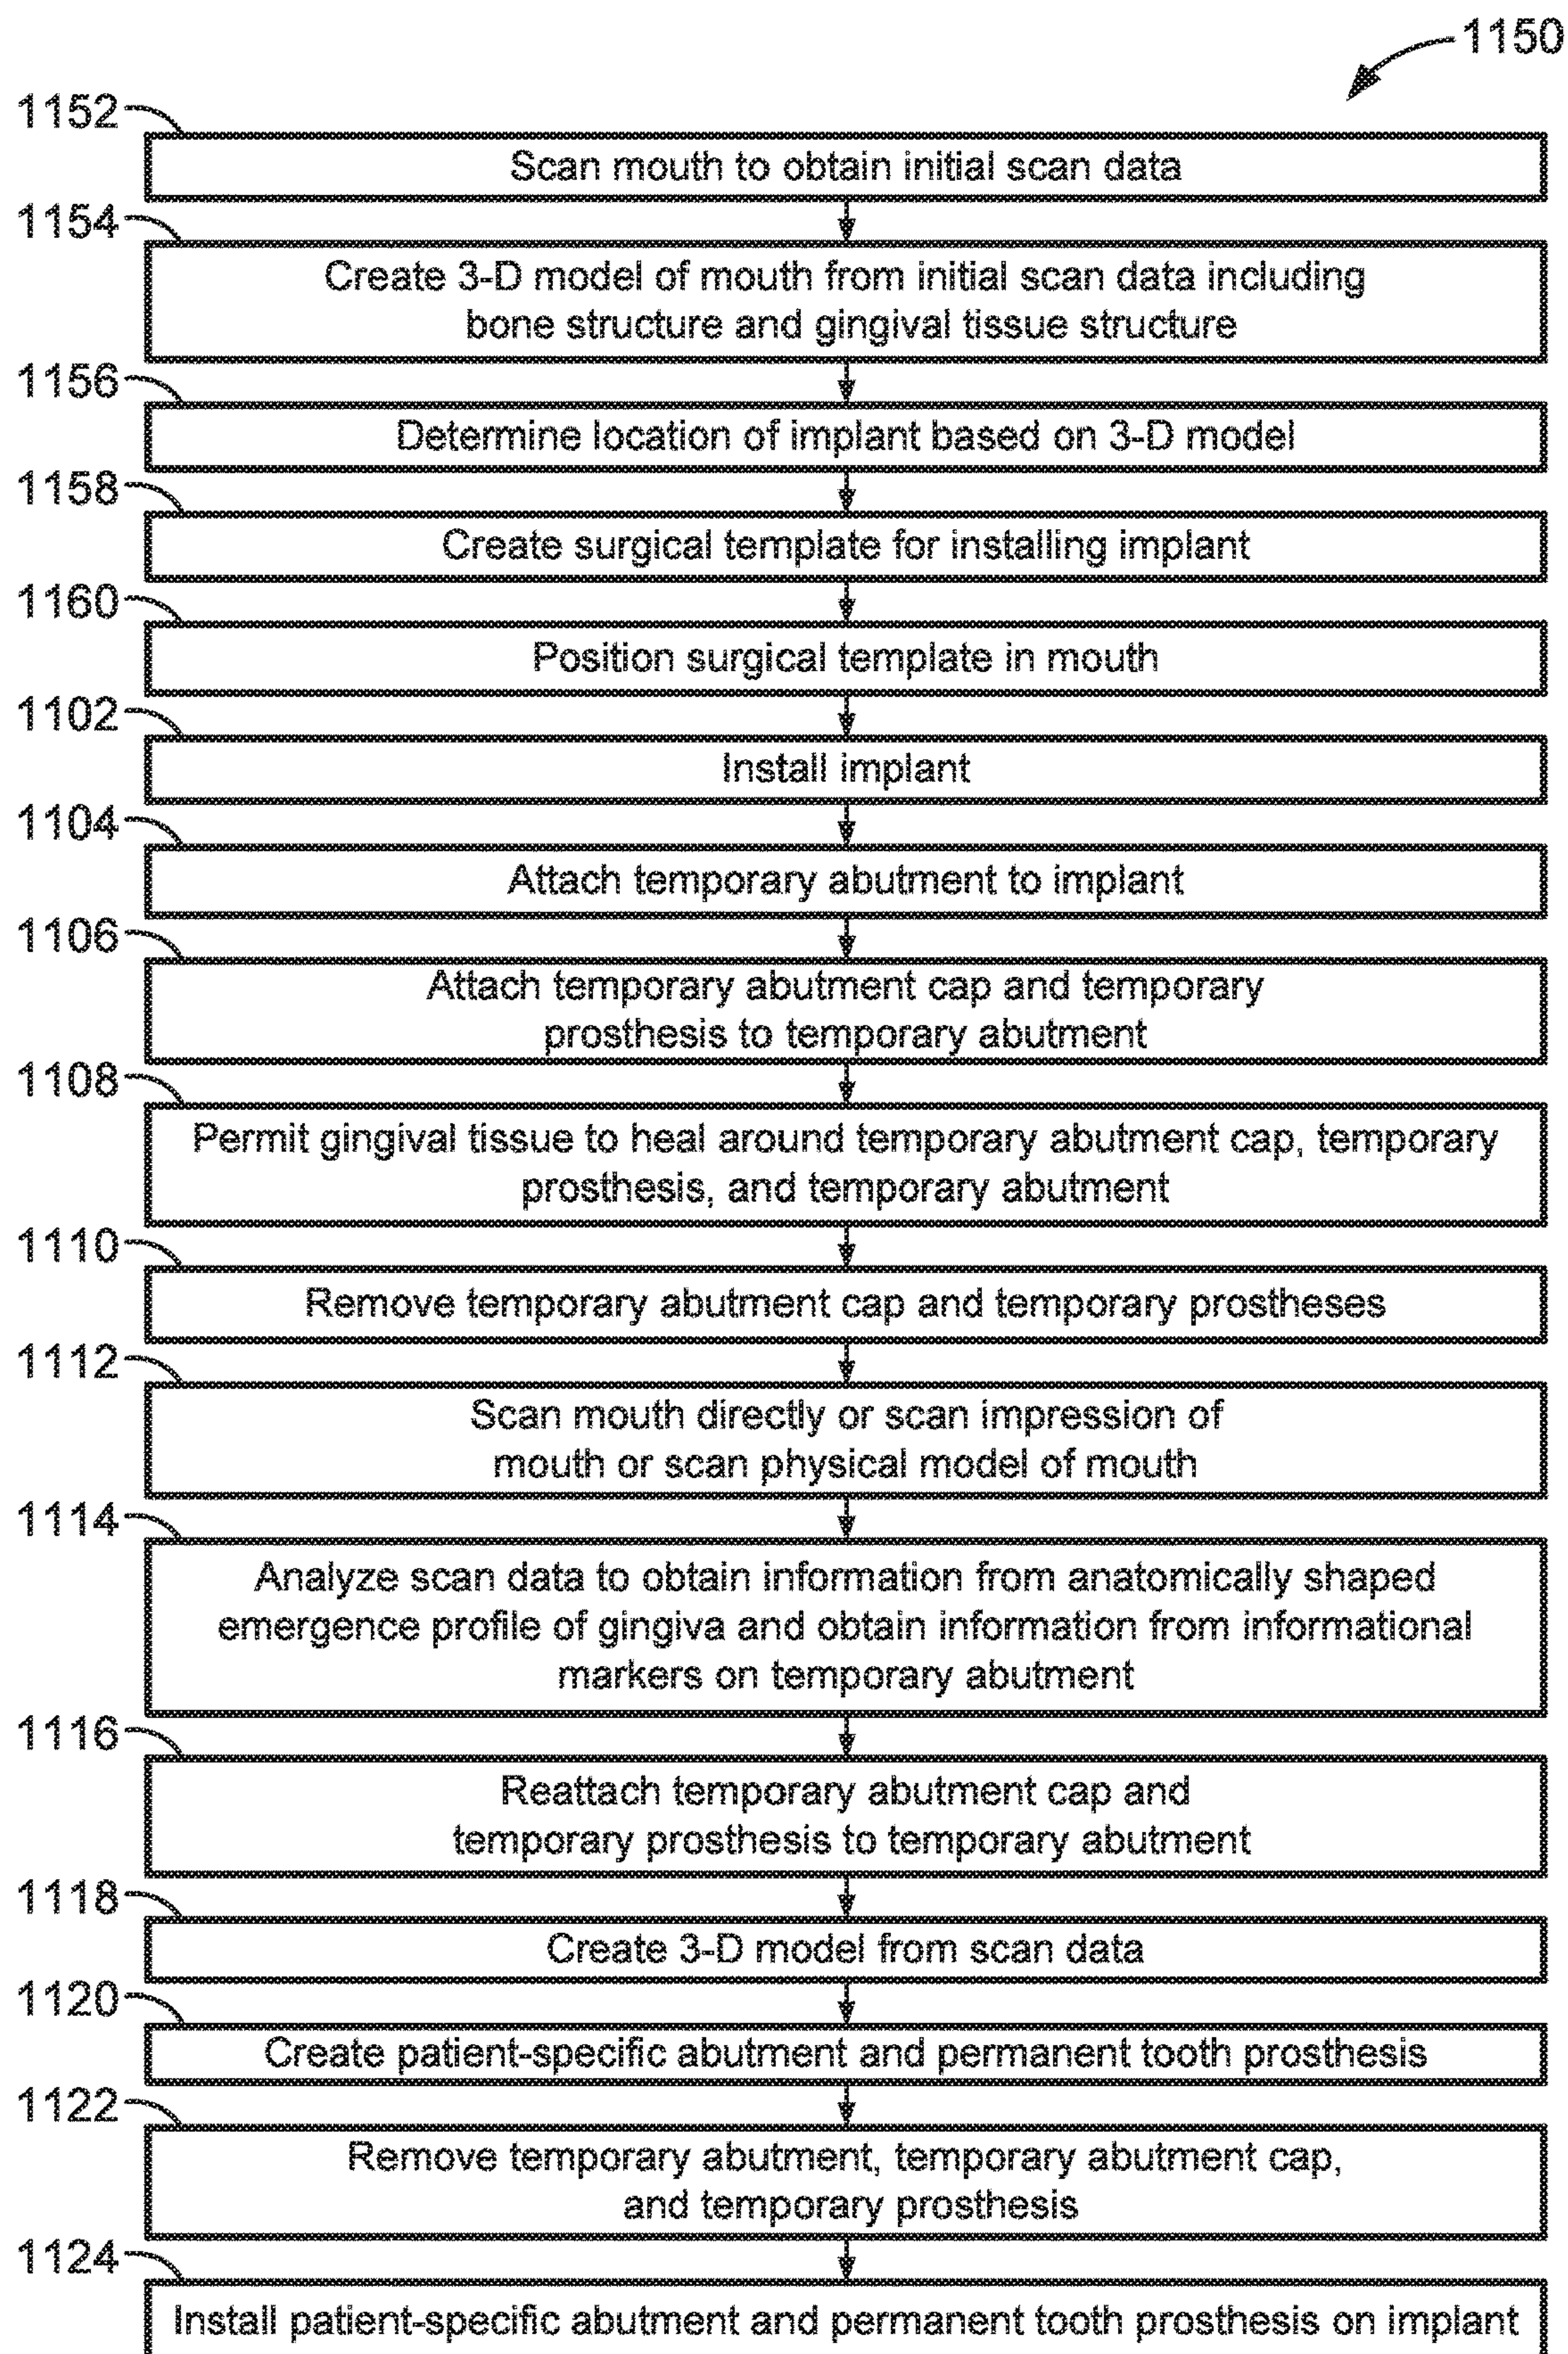


FIG. 16



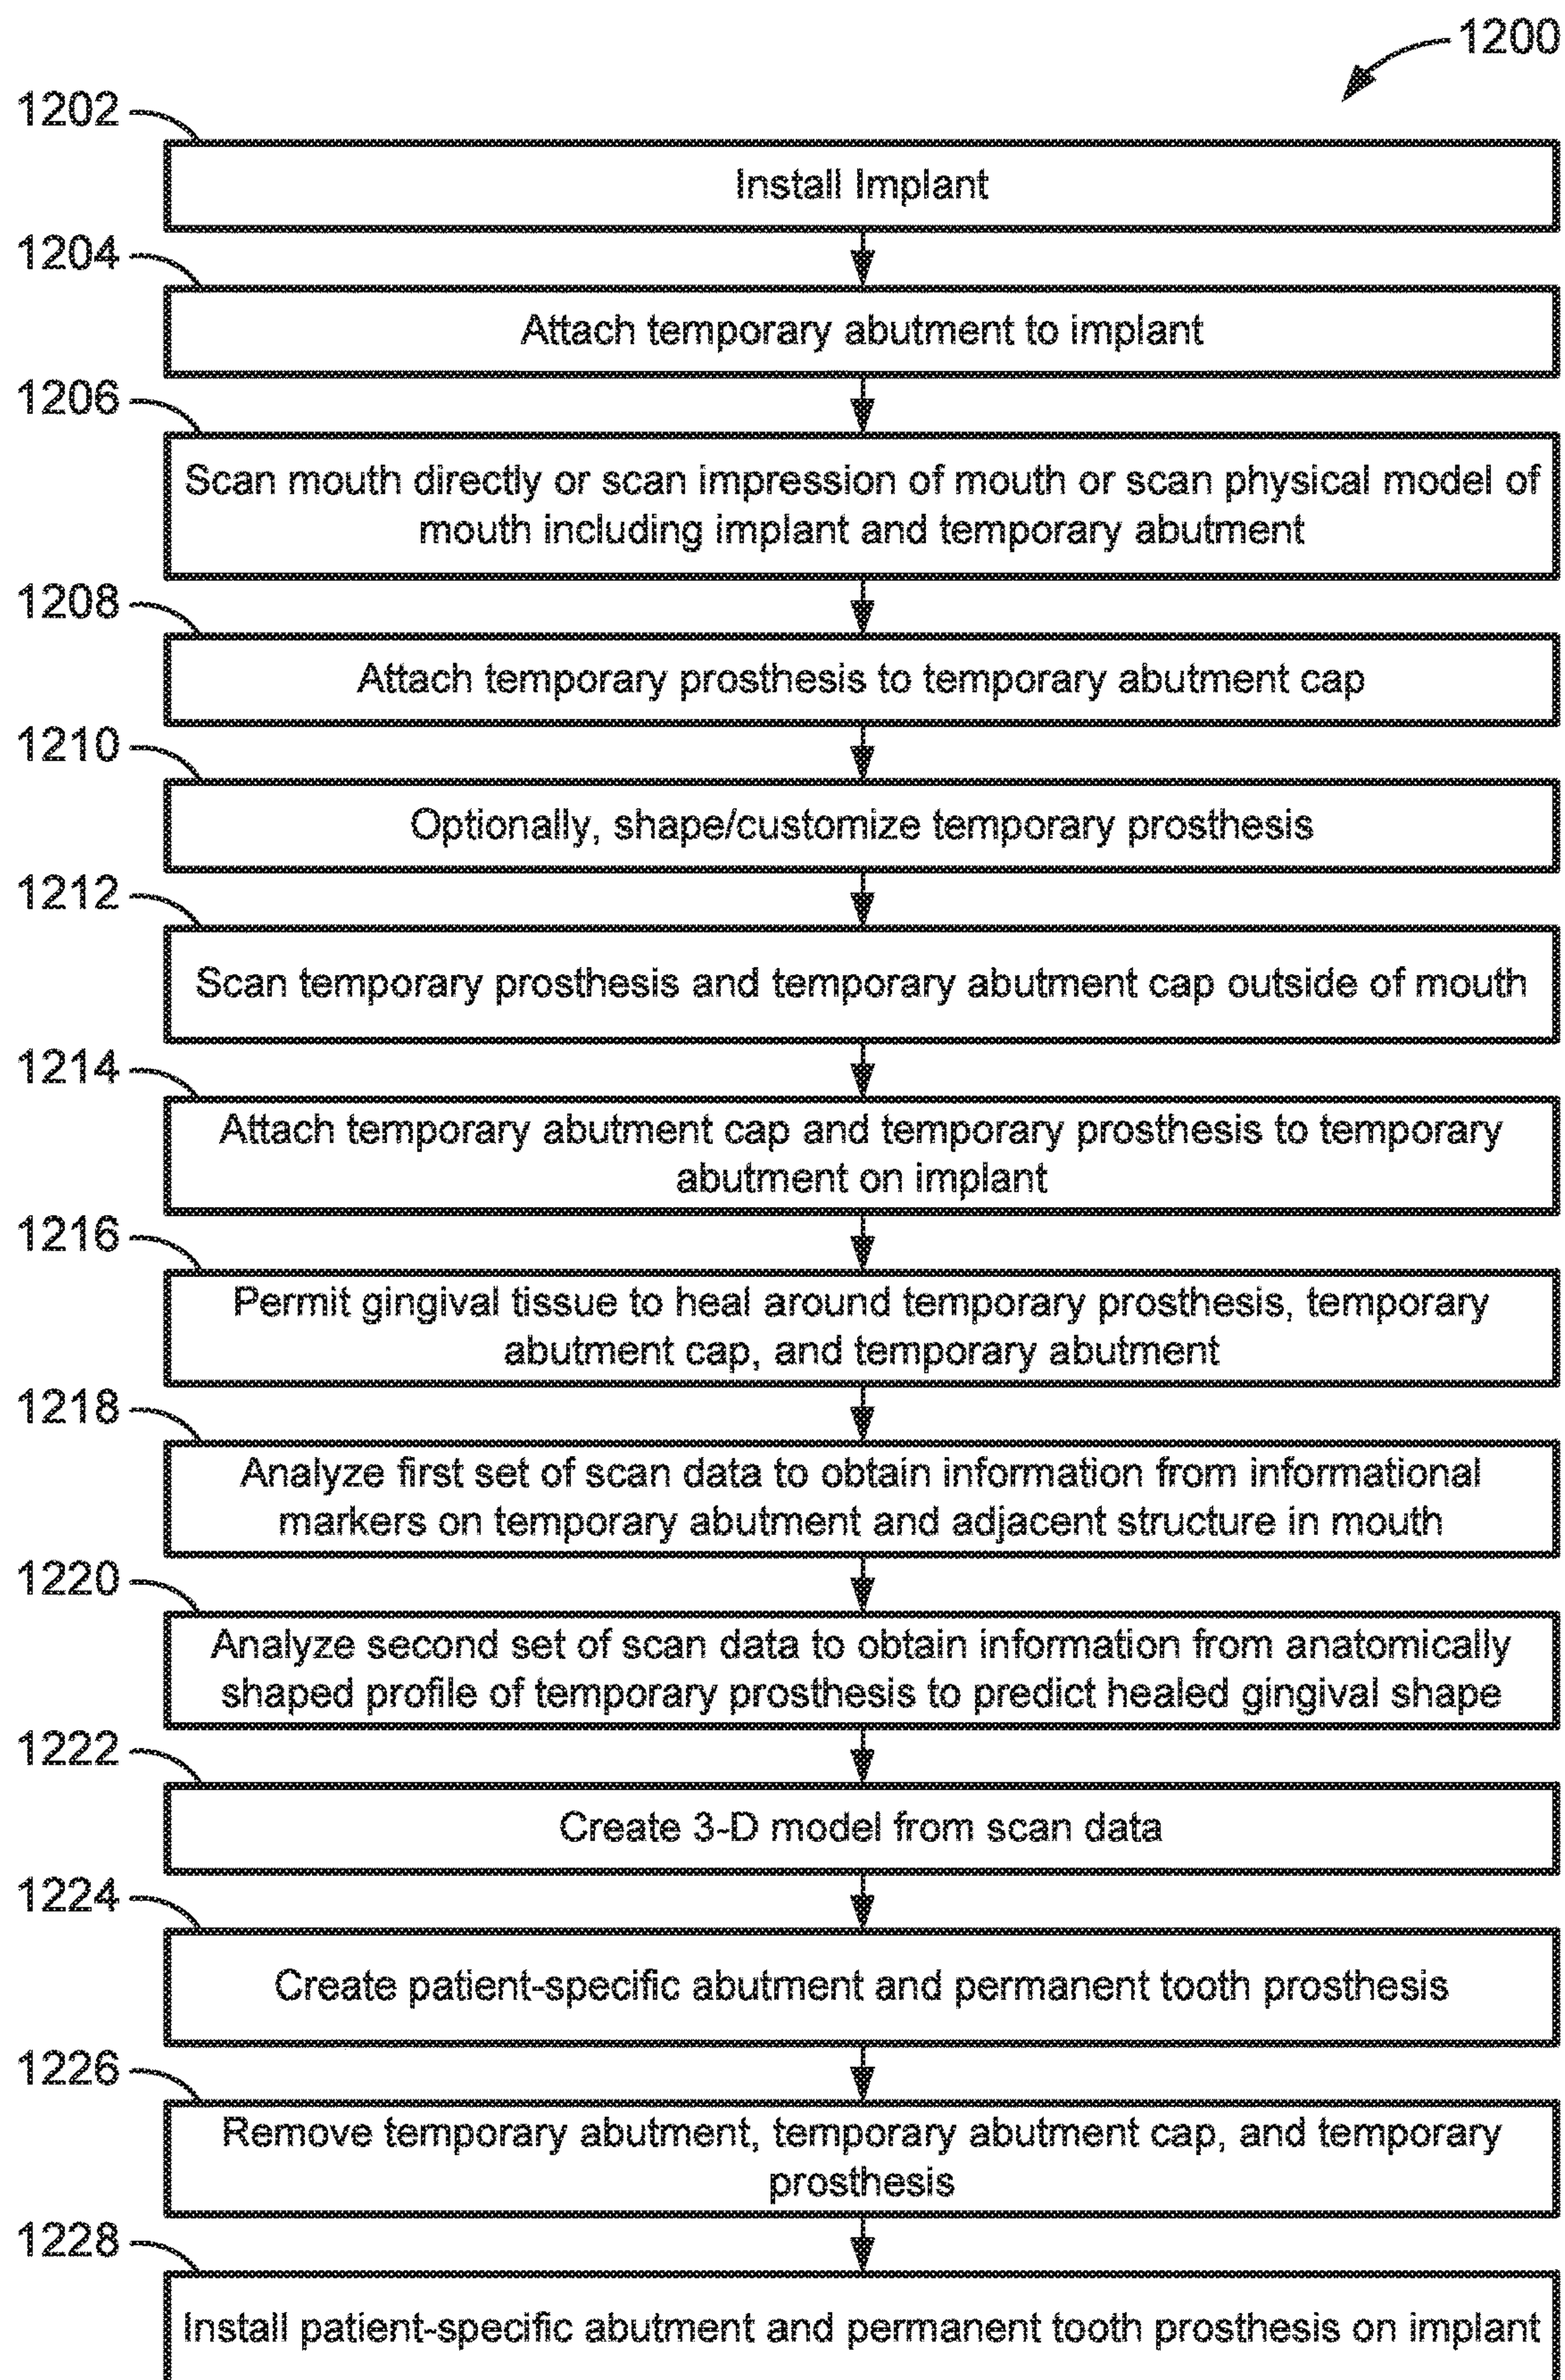


FIG. 17



# TEMPORARY ABUTMENT WITH COMBINATION OF SCANNING FEATURES AND PROVISIONALIZATION FEATURES

## CROSS-REFERENCE TO RELATED APPLICATION

This application is a continuation of prior application Ser. No. 14/575,717, filed Dec. 18, 2014 (now U.S. Pat. No. 10,368,964), which is a continuation of prior application Ser. No. 13/473,202, filed May 16, 2012, (now U.S. Pat. No. 8,944,816), which claims the benefit of U.S. Provisional Application Ser. No. 61/486,630, filed May 16, 2011 (now expired), each of which is hereby incorporated by reference herein in its entirety. This application is related to copending U.S. Ser. No. 13/473,219, filed on May 16, 2012, entitled "Temporary Abutment with Combination of Scanning Features and Provisionalization Features," (now U.S. Pat. No. 8,944,818).

## FIELD OF THE INVENTION

The present invention relates generally to a temporary abutment in a dental implant system. More particularly, the present invention relates to a temporary abutment having scanning features and provisionalization features.

## BACKGROUND OF THE INVENTION

The dental restoration of a partially or wholly edentulous patient with artificial dentition is typically done in two stages. In the first stage, an incision is made through the gingiva to expose the underlying bone. An artificial tooth root, in the form of a dental implant, is placed in the jawbone for osseointegration. The dental implant generally includes a threaded bore to receive a retaining screw for holding mating components thereon. During the first stage, the gum tissue overlying the implant is sutured and heals as the osseointegration process continues.

Once the osseointegration process is complete, the second stage is initiated. Here, the gingival tissue is re-opened to expose an end of the dental implant. A healing component or healing abutment is fastened to the exposed end of the dental implant to allow the gingival tissue to heal therearound. It should be noted that the healing abutment can be placed on the dental implant immediately after the implant has been installed and before osseointegration. In recent years, for some situations, the osseointegration step and gingival healing steps have been combined into a one-step process.

Prior healing abutments were generally round in profile, but the artificial teeth or prostheses that eventually replaced the healing abutments were not. Thus, the gingival tissue would heal around the healing abutments creating an emergence profile that approximated the size and contour of the healing abutment and not the size and contour of the prosthesis that was eventually attached to the implant. The resulting discrepancies between the emergence profile of the patient's gingiva and the installed prosthesis could sometimes require additional visits with the dentist or clinician to finalize the installation process and/or compromise the aesthetic outcome of the installed prosthesis. The present disclosure is directed to solving this and other problems with the prior healing abutments. There is also a need to resolve problems related to temporization of a prosthesis, as often times, prior to placing a permanent prosthesis, it is desirable to place a temporary prosthesis at the same location on the implant.

In more recent years, scanning technologies have been used to aid in the development of permanent prostheses. The present disclosure is also directed at solving problems with tying in the scanning technologies with the temporization of prostheses.

## SUMMARY OF THE INVENTION

An abutment assembly for attachment to a dental implant includes a temporary abutment and a temporary abutment cap. The temporary abutment has a lower region and an upper region. The lower region includes an anti-rotational feature for non-rotationally mating with the dental implant. The upper region includes a first anti-rotational structure and at least one retention groove. A top surface of the temporary abutment includes one or more informational markers that provide information concerning the dental implant. The temporary abutment cap is configured to be coupled to the upper region of the temporary abutment. The temporary abutment cap has at least one projection configured to mate with the at least one retention groove of the temporary abutment. The temporary abutment cap has a second anti-rotational structure that is configured to slidably engage the first anti-rotational structure of the temporary abutment. An outer surface of the temporary abutment cap is configured to be coupled with a temporary prosthesis such that the temporary prosthesis and the temporary abutment cap are removable from the temporary abutment lifting access to the informational markers.

A temporary prosthesis assembly for attachment to a dental implant includes a temporary abutment, a temporary abutment cap, and a temporary prosthesis. The temporary abutment includes an anti-rotational feature for non-rotationally mating with the dental implant. The temporary abutment includes one or more informational markers. The temporary abutment cap is configured to be removably coupled to the temporary abutment so as to cover the informational markers. The temporary prosthesis is configured to be coupled the temporary abutment cap. The combination of the temporary prosthesis and the temporary abutment cap is removably coupled to the temporary abutment.

An abutment for attachment to a dental implant includes a lower region, an upper region, and an internal bore. The lower region includes an anti-rotational feature for non-rotationally mating with the dental implant. The upper region includes an anti-rotational structure and at least one axial retention structure. The anti-rotational structure and the at least one axial retention structure is for engagement with a tooth-shaped prosthetic component. The upper region includes one or more informational markers for providing information concerning the dental implant that are revealed after the tooth-shaped prosthetic component has been removed from the abutment. The internal bore is configured to receive a fastening device for coupling the abutment to the dental implant.

A temporary abutment system for attachment to different types of dental implants includes a plurality of temporary abutments and a temporary abutment cap. Each of the temporary abutments includes a lower region and an upper region. The lower region includes an anti-rotational feature for non-rotationally mating with one of the dental implants. The upper region includes a first anti-rotational structure and a first axial retention structure. The upper region further includes informational markers for providing information concerning (i) the type of dental implant to which the temporary abutment is to be attached and (ii) positional or



3

dimensional information related to the attached dental implant. The temporary abutment cap has a second anti-rotational structure for mating with the first anti-rotational structure and a second axial retention structure for mating with the first axial retention structure. The temporary abutment cap is configured to be mated with any of the temporary abutments such that the temporary abutment cap covers the informational markers.

A method of creating a patient-specific abutment to be coupled to an implant installed in a mouth of a patient includes non-rotationally attaching a temporary abutment to the implant. The temporary abutment includes at least one informational marker indicative of one or more characteristics of the implant. A temporary prosthetic assembly is non-rotationally attached to the temporary abutment such that the temporary prosthetic assembly is removable therefrom. After a sufficient period of time during which gingival tissue surrounding the temporary prosthetic assembly has healed, the temporary prosthetic assembly is removed from the temporary abutment. After the removing, at least a portion of the mouth is scanned including the temporary abutment to generate scan data. From the scan data, emergence profile information for the gingival tissue adjacent to the temporary abutment is obtained and informational marker information from the temporary abutment is obtained. Based on the emergence profile information for the gingival tissue and the informational marker information, a three-dimensional model of at least a portion of the mouth is created. A patient-specific abutment is designed from the three-dimensional model.

A method of creating a patient-specific abutment to be coupled to an implant installed in a mouth of a patient includes attaching a non-round temporary prosthesis to the implant. The temporary prosthesis includes a temporary abutment that has at least one informational marker indicative of one or more characteristics of the implant. After gingival tissue surrounding the temporary prosthesis has healed in a non-round fashion, the temporary prosthesis is disassembled to expose the at least one informational marker on the temporary abutment without removing the temporary abutment from the implant. A scanning process is used to scan the at least one informational marker to obtain data including data associated with information about the implant. A patient-specific abutment is created from the data obtained via the scanning process.

A method of creating a patient-specific abutment to be coupled to an implant installed in a mouth of a patient includes non-rotationally attaching a temporary abutment to the dental implant. The temporary abutment includes at least one informational marker indicative of one or more characteristics of the implant. At least a portion of the mouth including the temporary abutment is scanned to generate a first set of scan data. After a shape for a temporary prosthesis has been selected, a temporary prosthesis is scanned outside of the mouth to generate a second set of scan data. The temporary prosthesis is attached to the temporary abutment such that the temporary prosthesis is removable therefrom. The first and the second sets of scan data is analyzed to obtain informational marker information and to obtain predicted anatomically shaped emergence gingiva profile information. A three-dimensional model of at least a portion of the mouth from the first and the second sets of scan data is created. A patient-specific abutment is designed from the three-dimensional model.

A method of creating a patient-specific abutment to be coupled to an implant installed in a mouth of a patient includes non-rotationally attaching a temporary abutment to

4

the implant. The temporary abutment includes at least one informational marker indicative of one or more characteristics of the implant. A temporary abutment cap is snap-fitted on the temporary abutment such that the temporary abutment cap is removable therefrom and at least partially obscures the at least one informational marker of the temporary abutment. A temporary prosthesis is attached to the temporary abutment cap. After a sufficient period of time during which gingival tissue surrounding the temporary prosthesis, the temporary abutment cap, and the temporary abutment has healed, the temporary prosthesis and the temporary abutment cap are removed from the temporary abutment. After the removing, at least a portion of the mouth is scanned including the temporary abutment to generate scan data. From the scan data, emergence profile information for the gingival tissue adjacent to the temporary abutment is obtained and informational marker information from the temporary abutment is obtained. Based on the emergence profile information for the gingival tissue and the informational marker information, a three-dimensional model of at least a portion of the mouth is created. A patient-specific abutment is designed from the three-dimensional model.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other advantages of the invention will become apparent upon reading the following detailed description and upon reference to the drawings.

FIG. 1A is a perspective view of a temporary abutment; FIG. 1B is a top view of the temporary abutment shown in FIG. 1A;

FIG. 2A is a perspective view of a second temporary abutment;

FIG. 2B is a top view of the second temporary abutment shown in FIG. 2A;

FIG. 3A is a perspective view of a fastening device used for holding the temporary abutments of the present disclosure on a dental implant;

FIG. 3B is a side cross-sectional view of the fastening device shown in FIG. 3A;

FIG. 4A is a perspective view of a temporary abutment cap;

FIG. 4B is a side view of the temporary abutment cap shown in FIG. 4A;

FIG. 5A is a perspective view of an abutment assembly;

FIG. 5B is a top cross-sectional view of the abutment assembly as shown in FIG. 5A;

FIG. 6A is an exploded cross-sectional view of a prosthesis assembly and a dental implant;

FIG. 6B is an assembled cross-sectional view of the prosthesis assembly coupled to the dental implant shown in FIG. 6A;

FIG. 7A is an exploded perspective view of an unmodified temporary abutment assembly including a temporary abutment, an unmodified temporary abutment cap, and a fastening device;

FIG. 7B is an assembled perspective view of the assembly shown in FIG. 7A with the temporary abutment cap modified;

FIG. 8A is an exploded perspective view of a prosthesis assembly and an implant according to an alternative embodiment of the invention;

FIG. 8B is a perspective view of a temporary abutment of the prosthesis assembly of FIG. 8A;

FIG. 8C is a perspective view of a screw of the prosthesis assembly of FIG. 8A;



## 5

FIG. 8D is a perspective view of a temporary abutment cap of the prosthesis assembly of FIG. 8A;

FIG. 8E is an exploded cross-sectional view of the prosthesis assembly and the implant of FIG. 8A;

FIG. 8F is an assembled cross-sectional view of the prosthesis assembly and the implant of FIG. 8A;

FIG. 9A is an exploded perspective view of a prosthesis assembly and an implant according to another alternative embodiment of the invention;

FIG. 9B is a perspective view of a temporary abutment of the prosthesis assembly of FIG. 9A;

FIG. 9C is a perspective view of a temporary abutment cap of the prosthesis assembly of FIG. 9A;

FIG. 9D is an exploded cross-sectional view of the prosthesis assembly and the implant of FIG. 9A;

FIG. 9E is an assembled cross-sectional view of the prosthesis assembly and the implant of FIG. 9A;

FIG. 10A is an exploded perspective view of a prosthesis assembly and an implant according to yet a further alternative embodiment of the invention;

FIG. 10B is a perspective view of a temporary abutment of the prosthesis assembly of FIG. 10A;

FIG. 10C is a perspective view of a temporary abutment cap of the prosthesis assembly of FIG. 10A;

FIG. 10D is an exploded cross-sectional of the prosthesis assembly and the implant of FIG. 10A;

FIG. 10E is an assembled cross-sectional view of the prosthesis assembly and the implant of FIG. 10A;

FIG. 11A is an exploded perspective view of a prosthesis assembly and an implant according to yet another alternative embodiment of the invention;

FIG. 11B is a perspective view of a temporary abutment of the prosthesis assembly of FIG. 11A;

FIG. 11C is a perspective view of a temporary abutment cap of the prosthesis assembly of FIG. 11A;

FIG. 11D is an exploded cross-sectional view of the prosthesis assembly and the implant of FIG. 11A;

FIG. 11E is an assembled cross-sectional view of the prosthesis assembly and the implant of FIG. 11A;

FIG. 12A is an exploded perspective view of a prosthesis assembly and an implant according to yet another alternative embodiment of the invention;

FIG. 12B is a perspective view of a temporary abutment of the prosthesis assembly of FIG. 12A;

FIG. 12C is a perspective view of a temporary abutment cap of the prosthesis assembly of FIG. 12A;

FIG. 12D is an exploded cross-sectional view of the prosthesis assembly and the implant of FIG. 12A;

FIG. 12E is an assembled cross-sectional view of the prosthesis assembly and the implant of FIG. 12A;

FIG. 13A is an exploded perspective view of a prosthesis assembly and an implant according to yet another alternative embodiment of the invention;

FIG. 13B is a perspective view of a temporary abutment of the prosthesis assembly of FIG. 13A;

FIG. 13C is a cross-sectional view of the temporary abutment of FIG. 13B;

FIG. 13D is a perspective view of a temporary abutment cap of the prosthesis assembly of FIG. 13A;

FIG. 13E is a cross-sectional view of the temporary abutment cap of FIG. 13D;

FIG. 13F is an exploded cross-sectional view of the prosthesis assembly and the implant of FIG. 13A;

FIG. 13G is an assembled cross-sectional view of the prosthesis assembly and the implant of FIG. 13A;

FIG. 13H is an assembled partial cross-sectional view of the prosthesis assembly and the implant of FIG. 13A;

## 6

FIG. 14A is an exploded perspective view of a prosthesis assembly and a dental implant according to yet another alternative embodiment of the invention;

FIG. 14B is an exploded perspective view of a prosthesis assembly and a dental implant according to yet another alternative embodiment of the invention;

FIG. 14C is an exploded perspective view of a prosthesis assembly and a dental implant according to yet another alternative embodiment of the invention;

FIG. 15 is a flow chart of a method for making a permanent patient-specific abutment and permanent tooth prosthesis using the prosthesis assembly components of the present invention;

FIG. 16 is a flow chart of a method for making a permanent patient-specific abutment and permanent tooth prosthesis including a method for preparing to install an implant; and

FIG. 17 is a flow chart of a method for making a permanent patient-specific abutment and permanent tooth prosthesis using the prosthesis assembly components of the present invention.

While the present disclosure is susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and will be described in detail herein. It should be understood, however, that the present disclosure is not intended to be limited to the particular forms disclosed. Rather, the present disclosure is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the present disclosure as defined by the appended claims.

#### DESCRIPTION OF ILLUSTRATIVE EMBODIMENTS

Retelling to FIGS. 1A and 1B, a temporary abutment 10 of the present disclosure (like other temporary abutments of the present disclosure) may be used for at least four purposes, which will be explained in more detail below. First, the temporary abutment 10 may serve as a gingival healing abutment as its exterior surface is contoured to aid in the healing of a patient's gingival tissue. Second, the temporary abutment 10 may serve as a temporary prosthesis (i.e., it provides a convenient mount for removably attaching an acrylic portion having an anatomical tooth shape). Third, the temporary abutment 10 serves as a scanning member to permit a clinician to use one or more scanning techniques to obtain necessary information about the underlying implant's location and orientation for use in developing permanent prosthetic components. And fourth, the temporary abutment 10 may serve as a permanent abutment providing a convenient mount for a permanent prosthesis having an anatomical tooth shape.

The temporary abutment 10 has a subgingival region 20 and a supragingival region 30, which are separated by a flange 50. An outer surface 55 (best shown in FIG. 5A) of the flange 50 is positioned to engage and aid in forming a patient's gingival tissue during the healing process. The subgingival region 20 includes an anti-rotational feature 22 (e.g., a hexagonal section) for mating with a corresponding anti-rotational feature of an implant (e.g., implant 120 in FIG. 6A). The anti-rotational feature 22 of the temporary abutment 10 can be any type of boss (e.g., polygonal boss, star boss, clover boss, etc.) or socket (e.g., polygonal socket, star socket, clover socket, etc.) such that it corresponds with an anti-rotational feature of the underlying implant to prevent relative rotation of the temporary abutment 10 with respect to the implant 120. It is contemplated that the



temporary abutment 10 (and the other temporary abutments of the present disclosure) can be fashioned from gold, titanium, plastic, ceramic, or other similar metals or composites.

The supragingival region 30 includes one or more retention grooves or structures 32 and an anti-rotational structure 34 (e.g., a flat wall or surface). The retention grooves 32 are configured to mate in a snap-type axial holding engagement with corresponding male circumferential features or structures 86 (shown in FIGS. 4A and 4B) of a temporary abutment cap 80 (shown in FIGS. 4A and 4B). The one or more retention grooves 32 are configured to mate with the male circumferential features 86 with a retention force between about one and about ten pounds of force. That is, it takes between about one and about ten pounds of force to remove the temporary abutment cap 80 from its snap-fit type engagement with the temporary abutment 10. Alternatively, the supragingival region 30 of the temporary abutment 10 can include male circumferential features that are configured to mate in a snap-type axial holding engagement with corresponding retention grooves on an inside surface of the temporary abutment cap 80 (not shown).

The anti-rotational structure 34 is configured to mate in a slidable engagement with a corresponding anti-rotational structure 84 (shown in FIGS. 4A and 4B) to prevent relative rotation of the temporary abutment cap 80 and the temporary abutment 10. In the illustrated implementation, the anti-rotational structure 34 generally extends from a top surface 60 of the temporary abutment 10 to the flange 50. While the anti-rotational structure 34 is shown as a flat wall on the supragingival region 30, the anti-rotational structure 34 can be one of a variety of known anti-rotational structures, such as, for example, one or more grooves, slots, projections, or any combination thereof. Examples of anti-rotational structures for dental posts are shown in U.S. Pat. Nos. 6,120,293, 6,159,010, and 8,002,547, each of which is commonly owned by the assignee of the present application and is hereby incorporated by reference herein in its entirety. Regardless of the type of anti-rotational structure 34 chosen for the supragingival region 30 of the temporary abutment 10, the temporary abutment cap 80 has a correspondingly shaped structural surface (e.g., anti-rotational structure 84) for engaging the anti-rotational structure 34 so as to prevent relative rotation between the two components.

The temporary abutment 10 is generally cylindrical in shape with an internal bore 40 for receiving a screw 70 (shown in FIGS. 3A and 3B) to removably couple the temporary abutment 10 to the implant 120. The top surface 60, which is best shown in FIG. 1B, includes two informational marker locations 62. The informational marker locations 62 are positioned circumferentially around the top surface 60 of the temporary abutment 10. While the temporary abutment 10 is shown with informational marker locations 62 only at locations of 3 o'clock, and 6 o'clock with respect to the anti-rotational structure 34 being at 12 o'clock, it is contemplated that additional informational marker locations (not shown) can be placed at 9 o'clock, 12 o'clock, and/or at any positions therebetween.

Each of the informational marker locations 62 is configured to include one or more informational markers 64. The informational marker 64 is shown as one notch; however, the present disclosure contemplates that the informational markers 64—for all of the embodiments disclosed herein—can be positive informational markers, negative informational markers, raised projections/pimples, recesses or dimples, notches, lines, etching, alphanumeric characters, etc. It is further contemplated that the cross-section of the informa-

tional markers 64 can be rectangular, triangular, or various other shapes. Further, the informational marker locations 62 themselves can act as informational markers and provide and/or indicate information.

The informational markers 64 are indicative of one or more characteristics of the temporary abutment 10 itself and/or of the underlying implant 120 (shown in FIG. 6A) to which the temporary abutment 10 is attached. For example, one or more of the informational markers 64 can be geometrically aligned with a flat of the non-rotational feature 22 of the temporary abutment 10 and/or a flat on the underlying implant to indicate the rotational orientation of the non-rotational features of the temporary abutment 10 and/or of the underlying implant. It is also contemplated that one or more of the informational markers 64 may correspond to the height of the temporary abutment 10 and, hence, a height or vertical position (i.e., z-axis location) of a table or seating surface of the underlying implant. For another example, the informational markers 64 can be indicative of the x-y location of the table or seating surface of the underlying implant. For another example, the informational markers 64 can be indicative of the angle that the underlying implant rests with respect to vertical within the patient's jawbone (e.g., pitch and yaw). For another example, the informational markers 64 can be indicative of the size and/or shape of the temporary abutment 10 and/or the underlying implant. For another example, the informational markers 64 can be indicative of the manufacturer of the underlying implant.

The informational markers 64 can be part of a binary marking system that identifies unique characteristics of the temporary abutment 10 and/or the underlying implant 120. As is well known, a binary-coded system exists as an array of digits, where the digits are either "1" or "0" that represent two states, respectively, ON and OFF. For each informational marking location 62, the presence of an informational marker 64 ("ON") is a 1 and the absence of an informational marker 64 ("OFF") is a 0. By grouping sets of 1's and 0's together starting from a known starting location (e.g., 3 o'clock or the first location in the clockwise direction from the anti-rotational structure 34), information about each temporary abutment 10 is known. For the temporary abutment 10, the two informational marker locations 62 can provide four different combinations. Additional details on informational markers and the characteristics of the underlying implant and/or the abutment that are identified by the informational markers (e.g., informational markers 64) can be found in U.S. Pat. No. 7,988,449, which is hereby incorporated by reference herein in its entirety.

Referring to FIGS. 2A and 2B, a temporary abutment 10' is shown. The temporary abutment 10' includes all of the same features as the temporary abutment 10, where like reference numbers are used for like components; however, the temporary abutment 10' is a different size of temporary abutment. The difference is noticeable by reference to the orientation or positioning of the informational marker 64' and the informational marker locations 62' on the top surface 60 of the temporary abutment 10'. A quick comparison of the top surface 60 of the temporary abutment 10' reveals that the informational marker 64' is in a different orientation, which indicates that the temporary abutment 10' has at least one characteristic that is different from the temporary abutment 10. For example, the temporary abutment 10' has a larger or wider subgingival region 20 and flange 50 than the subgingival region 20 and flange 50 of the temporary abutment 10. For another example, the outer surface 55 of the flange 50



of the temporary abutment 10' can have a different curve and/or profile than the outer surface 55 of the flange 50 of the temporary abutment 10.

Referring to FIGS. 3A and 3B, a fastening device such as the screw or attaching bolt 70 includes a threaded portion 72, a shaft portion 74, and a head portion 76 including a socket. The head portion 76 on the exposed surface of a head of the screw 70 is shaped to accept a wrench (not shown) for threadably engaging the screw 70 into a threaded bore of an implant 120 (shown in FIG. 6A). It is contemplated that each of the temporary abutments described herein and shown in the figures can be secured to an implant by means of the screw 70, or by means of a similar screw, as is known in the art. It is further contemplated that one or more washers (e.g., locking washer) and/or O-rings (e.g., sealing O-ring) can be placed on the screw 70 (e.g., below the head portion 76 on the shaft portion 74 and/or about or on the head portion 76) prior to installation of the same. While not shown in FIGS. 3A and 3B, the head portion 76 of the screw 70 can include one or more informational marker locations and/or informational markers that are the same as, or similar to, the informational marker locations 62 and the informational markers 64 described above in reference to the temporary abutment 10 (see e.g., notches 478 of screw 470 in FIG. 8C). Such informational markers on the screw 70 can provide and/or be indicative of information such as, for example, a connection type of the underlying implant (e.g., implant 120 of FIG. 6A), a manufacturer of the underlying implant, a height, a width, a pitch, a yaw, or a combination thereof, of the screw 70 itself, of the temporary abutment 10, and/or of the underlying implant.

Now referring to FIGS. 4A and 4B, the temporary abutment cap 80 has a generally cylindrical outer surface 81 (or it could have a slight taper) and is configured to fit over the supragingival region 30 of the temporary abutment 10 after the screw 70 is installed. Alternatively, it is contemplated that the temporary abutment cap 80 includes an aperture (see e.g., aperture 483 in temporary abutment cap 480 in FIG. 8D) in a top portion thereof to provide access for the screw 70 to be installed after the temporary abutment cap 80 is installed on the temporary abutment 10.

The temporary abutment cap 80 includes an anti-rotational structure 84 that projects inward from an inner surface 82 of the temporary abutment cap 80. The anti-rotational structure 84 is configured to engage with and/or abut the anti-rotational structure 34 of the temporary abutment 10 in a slidable manner as the temporary abutment cap 80 is slid over the temporary abutment 10. The outer dimensions (e.g., diameter) of the supragingival region 30 of the temporary abutment 10 and the inner dimensions of the inner surface 82 of the temporary abutment cap 80 are configured such that the temporary abutment cap 80 can be slid over the supragingival region 30 in only one rotational orientation. Such a design prevents the temporary abutment cap 80 from rotating with respect to the supragingival region 30 of the temporary abutment 10 once installed. It is contemplated that the temporary abutment cap 80 can include more than one anti-rotational structure 84 configured to mate with a corresponding number of anti-rotational structures 34 of the temporary abutment 10.

The temporary abutment cap 80 includes one or more male circumferential features 86 that are configured to mate with the temporary abutment 10 in a snap-fit type engagement. The one or more male circumferential features 86 are circumferential projections that mate with corresponding ones of the retention grooves 32 on the supragingival region 30 of the temporary abutment 10. Such a mating of the male

circumferential features 86 with the retention grooves 32 removably couples the temporary abutment cap 80 to the temporary abutment 10. It is contemplated that such a removable snap-fit type engagement provides a clinician installing the temporary abutment cap 80 with mechanical and/or audible feedback that a bottom end 88 (FIG. 4A) of the temporary abutment cap 80 is properly seated on the flange 50 (FIG. 1A) of the temporary abutment 10.

Now referring to FIGS. 5A and 5B, an abutment assembly 85 includes the temporary abutment 10 engaged with the temporary abutment cap 80 in a snap-fit type engagement. As shown in FIG. 5A, the temporary abutment cap 80 is installed on the temporary abutment 10 such that the bottom end 88 (FIG. 4A) of the temporary abutment cap 80 abuts and/or contacts the flange 50 (FIGS. 1A and 1B) of the temporary abutment 10 and the male circumferential projections 86 (FIGS. 4A and 4B) of the temporary abutment cap 80 engage the retention grooves 32 (FIGS. 1A and 1B) of the temporary abutment 10. As shown in FIG. 5B, the anti-rotational structure 34 of the temporary abutment 10 is positioned adjacent to the anti-rotational structure 84.

Referring to FIGS. 6A and 6B, an exploded view (FIG. 6A) and an assembled view (FIG. 6B) of a temporary prosthesis assembly or a prosthesis assembly 100 and dental implant 120 is shown. The prosthesis assembly 100 includes the temporary abutment 10 and the temporary abutment cap 80 coupled to a temporary prosthesis 90 (e.g., a temporary tooth). The implant 120 is installed in the jawbone (not shown) of a patient, and then the temporary abutment 10 is non-rotationally attached to the implant 120 via the non-rotational feature 22 and the screw 70. The temporary abutment 10 is attached to the implant 120 such that a bottom portion of the flange 50 of the temporary abutment 10 abuts and/or rests upon a table or seating surface 123 of the dental implant 120. The temporary abutment cap 80 is snap-fitted onto the temporary abutment 10 and then the temporary prosthesis 90 is coupled to the temporary abutment cap 80.

The outer surface 81 of the temporary abutment cap 80 is configured to mate with and/or to be bonded with the temporary prosthesis 90. It is contemplated that the temporary prosthesis 90 is coupled to the temporary abutment cap 80 using cement (e.g., dental cement), glue, bonding agent, a press-fit engagement, a snap or click-type engagement, a screw or bolt, or a combination thereof. It is further contemplated that the temporary prosthesis 90 is removably or permanently coupled to the temporary abutment cap 80 such that the temporary prosthesis 90 and the temporary abutment cap 80 can be removed separately or in unison from the temporary abutment 10. Removal of the temporary prosthesis 90 and the temporary abutment cap 80 exposes the top surface of the temporary abutment 10 including the informational markers 64, which can be scanned directly or indirectly (e.g., from an impression and/or stone/plaster model) to generate scan data that is at least used to determine the location and orientation of the implant 120, which, as explained herein, is used when developing a permanent patient-specific abutment and/or prosthesis.

The outer surface of the temporary prosthesis 90 and/or the outer surface 55 of the flange 50 are configured to be suitable for replicating the gingival emergence profile formed by a natural tooth (e.g., in a non-round shape). As such, after the temporary prosthesis 90 is installed, the patient's gingiva is permitted to heal around the temporary prosthesis 90 and/or the temporary abutment 10. Such a prosthesis assembly 100 results in a gingival emergence profile approximating that of what would be around a natural



## 11

tooth and/or that of what a clinician determined to be most appropriate for the given implant installation site (e.g., an ovular shape). In other words, the prosthesis assembly **100** also acts as a gingival healing abutment. This is advantageous because, after the patient's mouth has an opportunity to heal and is ready to be processed (e.g., intra-oral direct scanning, impression scanning, or scanning of a model formed from the impression) for creating a permanent patient-specific abutment and prosthesis, the temporary prosthesis **90** and the temporary abutment cap **80** are removed to reveal the temporary abutment **10** and the resulting emergence profile of the adjacent gingiva. Because the resulting emergence profile approximates that of a natural tooth, the permanent patient-specific abutment and prosthesis can be accurately created from the scan data and/or from known data associated with the temporary abutment **10** (e.g., the known contours of the outer surface **55** of the flange **50** of the temporary abutment **10**). For example, the permanent patient-specific abutment and prosthesis can be created and attached to the underlying implant **120** such that the permanent patient-specific abutment and prosthesis (not shown) are highly aesthetic and fit closely within the gingiva emergence profile adjacent to the implant **120** that was formed by the prosthesis assembly **100**.

To create a permanent patient-specific abutment and prosthesis (not shown), after the temporary abutment cap **80** and attached temporary prosthesis **90** are removed, the dental region of the patient's mouth including the temporary abutment **10** is scanned from a stone model (i.e., a replica of the patient's dental conditions), from impression material of an impression of the patient's dental conditions including the temporary abutment **10**, or directly in the mouth of the patient. Scanning can be accomplished using a laser scanning technique, a photographic scanning technique, or a mechanical sensing technique. These methods of scanning directly in a patient's mouth, an impression of the same, and a model of the same, using any of the aforementioned techniques, are described in further detail in U.S. Pat. No. 7,988,449, which was previously incorporated by reference herein in its entirety.

The scanned data or information obtained from the scanning process is then transferred to a graphical imaging program for analysis. The graphical imaging software program, due to the information markers **64** on the top surface **60** of the temporary abutment **10**, can aid in performing a wide variety of functions. For example, the graphical imaging program can scan an opposing cast in order to develop an opposing occlusal scheme and relate this information back to the primary model. This feature is extremely important because many clinical patients have implants in both maxillary and mandibular locations. Each of the features of the temporary abutment **10** and underlying implant **120** is analyzed and determined based on the presence/absence of the information markers **64** and the orientation/location of the informational markers **64** on the top surface **60** of the temporary abutment **10**. And, as mentioned above, the emergence contour or profile of the gingival tissue that was created by the prosthesis assembly **100** is also received in the scan.

Final dimensional information determined by the graphical imaging computer program is transferred from the computer to a milling machine (e.g., a 5 axis milling machine) to fabricate the permanent patient-specific abutment and/or permanent prosthesis. It is contemplated that the permanent patient-specific abutment and/or permanent prosthesis can be fashioned from gold, titanium, plastic, ceramic, or other similar metals or composites.

## 12

Alternatively and/or additionally, one or more rapid prototype models of the patient's mouth, including a replica of the gingival contours, can be fabricated based on the dimensional information and/or the original scanned information/data. The rapid prototype model(s) can be used by a clinician to develop, for example, the permanent prosthesis. Additional details on rapid prototype models and rapid prototyping in general can be found in U.S. Pat. No. 8,185,224, which is hereby incorporated by reference herein in its entirety.

FIGS. 7A-7B illustrate an alternative abutment assembly **200**. FIG. 7A shows an exploded view of the abutment assembly **200** including the temporary abutment **10** and a temporary abutment cap **280**. The temporary abutment cap **280** is configured to be installed on the temporary abutment **10** such that (1) a bottom end **288** of the temporary abutment cap **280** abuts and/or contacts a top portion of the flange **50** of the temporary abutment **10** and (2) male circumferential projections **286** of the temporary abutment cap **280** engage the retention grooves **32** of the temporary abutment **10** in a snap-fit type engagement.

The temporary abutment cap **280** is similar to the temporary abutment cap **80**, described herein and shown in FIGS. 4A and 4B, except that the temporary abutment cap **280** includes additional material **282** configured to be cut or shaved or otherwise modified by a clinician to approximate the size, shape, position, and general likeness of an anatomically shaped tooth when attached to the temporary abutment **10**. For example, as shown in FIG. 7B, the additional material **282** of the temporary abutment cap **280** is modified to look like an anatomically shaped tooth when attached to the temporary abutment **10** installed on the dental implant **120** (not shown in FIG. 7B) in the mouth of a patient. The embodiment of FIGS. 7A and 7B is different from FIGS. 4A and 4B in which material (e.g., the temporary prosthesis **90**) is added to the temporary abutment cap **80** to form the emergence profile of the gingival tissue.

Alternatively, the additional material **282** can be modified such that the modified portion of the temporary abutment cap **280** is configured to be coupled with a temporary prosthesis or crown (not shown) in a manner similar to how the temporary prosthesis **90** is coupled to the temporary abutment cap **80**, described above and shown in FIGS. 6A and 6B.

According to some additional alternative implementations of the present aspects, in lieu of a clinician modifying the additional material **282** of the temporary abutment cap **280**, a temporary abutment cap can be supplied with a shape and size such that the temporary abutment cap includes an outer surface that approximates the size and shape of an anatomically shaped tooth when attached to the temporary abutment **10** installed on the dental implant **120** in the mouth of a patient. That is, it is contemplated that a temporary abutment cap can be formed with an outer surface that includes a preformed anatomically shaped tooth (e.g., a tooth prosthesis) that is configured to be attached to the temporary abutment **10** in a similar manner as the temporary abutment cap **80** is attached to the temporary abutment **10** described herein.

It is further contemplated that a kit or package of temporary abutment caps, where each temporary abutment cap includes an outer surface with an anatomically shaped tooth (not shown), can be supplied and/or packaged together for use by, for example, clinicians. In such alternatives, the clinician is supplied with a variety of temporary abutment caps including different anatomically shaped teeth that can be attached to the temporary abutment **10** as described



herein and used directly as temporary prostheses without further modification or attachment of additional components. In each of these alternatives, the temporary abutment 10 is still useful for scanning.

In some implementations of the disclosed concepts, the retention grooves 32 and the male circumferential features 86 can be formed to provide a fixed rotational orientation between the temporary abutment 10, 10' and the temporary abutment cap 80. For example, one or more of the retention grooves 32 can have a unique length and/or size (as compared with the other ones of the retention grooves 32) that is designed to mate with a corresponding one of the male circumferential features 86 having a corresponding unique length and/or size (as compared with the other ones of the male circumferential features 86) such that the temporary abutment cap 80 can only be attached (e.g., via snap-fit connection) to the temporary abutment 10, 10' in one rotational orientation.

Referring to FIGS. 8A to 8F, various views of components of an alternative prosthesis assembly 400 and the dental implant 120 are shown. As shown in FIG. 8A, the prosthesis assembly 400 includes a temporary abutment 410, a temporary abutment cap 480, a screw 470, and a temporary prosthesis 490, each of which is similar to, or the same as, corresponding components of the previously described prosthesis assemblies. In FIGS. 8A to 8F, each of the components and features is identified by a 400-series reference numeral, and those 400-series reference numerals correspond to like features of the various components and features of the previously described prosthesis assemblies. For example, reference numeral 434 is used to describe the non-rotational structure 434 (FIG. 8B), which is the same as, or similar to, the non-rotational structure 34 (FIG. 1A). Additionally, reference numerals 440, 460, 472, 474, and 481 are used in the figures to illustrate features that are the same as, or similar to, previously described features with reference numbers 40, 60, 72, 74, and 81, respectively.

Referring to FIG. 8B, the temporary abutment 410 generally includes all of the same features as the temporary abutment 10, which is most similar to the temporary abutment 410; however, the temporary abutment 410 has a different overall shape and/or size. Specifically, the temporary abutment 410 includes a continuous retention groove 432 that circumscribes the entire supragingival region 430 of the temporary abutment 410 instead of including the retention grooves 32 (FIG. 1A) of the temporary abutment 10. Additionally, the continuous retention groove 432 (FIG. 8B) is positioned completely below the non-rotational structure 434 of the temporary abutment 410 as compared to the positioning of the retention grooves 32 of the temporary abutment 10 which are positioned adjacent to a central region of the non-rotational structure 34 of the temporary abutment 10 (e.g., the retention grooves 32 are relatively higher on the temporary abutment 10). Irrespective of the placement of the continuous retention groove 432 on the supragingival region 430 of the temporary abutment 410, the continuous retention groove 432 (FIG. 8B) functions in the same, or similar, manner as the retention grooves 32 (FIG. 1A) in that the continuous retention groove 432 is configured to mate with one or more projections 486 of the temporary abutment cap 480 (FIG. 8D) in a snap-fit type engagement (shown in FIG. 8F).

An outer surface 455 of a flange 450 of the temporary abutment 410 (e.g., portion of 410 that separates a subgingival region 420 and a supragingival region 430) also differs from the outer surface 55 of the flange 50 of the temporary abutment 10, which is best seen by comparing FIG. 6B with

FIG. 8F. Specifically, the outer surface 455 of the flange 450 of the temporary abutment 410 has a differently shaped contour for engaging and aiding in forming a patient's gingival tissue during the healing process. Various other contours of the outer surface 455 of the flange 450 can be used depending on the particular conditions present in the patient's mouth.

A further difference between the temporary abutment 410 (FIG. 8B) and the temporary abutment 10 (FIG. 1A) is that the temporary abutment 410 includes three informational marker locations 462 and two informational markers 464 as compared to the two informational marker locations 62 and the one informational marker 64 of the temporary abutment 10. The additional informational marker location 462 can aid in providing additional information about the temporary abutment 410 and/or the underlying dental implant 120 by providing, for example, additional potential binary combinations (e.g., three binary informational markers provide the ability to identify eight different configurations).

Referring to FIG. 8C, the screw 470 generally includes all of the same features as the screw 70; however, an upper part of a head portion 476 of the screw 470 is modified. Specifically, in addition to the head portion 476 including a socket 479 to accept a wrench (not shown) for threadably engaging the screw 470 into the threaded bore of the implant 120 (see FIGS. 8A, 8E, and 8F), the head portion 476 includes a lip 477 and one or more notches 478.

The lip 477 has a larger outer diameter than the outer diameter of the rest of the head portion 476 such that the lip 477 engages with the temporary abutment cap 480 when the temporary abutment cap 480 is engaged with (e.g., snapped onto) the temporary abutment 410 as best shown in FIG. 8F. Such an engagement between the lip 477 and the temporary abutment cap 480 provides additional rigidity to the prosthesis assembly 400 in its assembled configuration (FIG. 8F). Alternatively, the screw 470 can be sized and shaped such that the head portion 476 does not engage the temporary abutment cap 480 (see e.g., FIG. 6B).

The one or more notches 478 in the head portion 476 can act as informational marker locations and/or informational markers in the same, or similar, manner as the informational marker locations 62, 462 and the informational markers 64, 464 described herein. Specifically, the notches 478 can indicate information regarding one or more aspects of the prosthesis assembly 400 and/or the dental implant 120, such as, for example, a connection type of the underlying implant, the type of prosthesis assembly, a manufacturer of the underlying implant, a height, a width, a pitch, a yaw, or a combination thereof of the temporary abutment 410 and/or of the underlying implant 120, etc.

Referring to FIG. 8D, the temporary abutment cap 480 generally includes all of the same features as the temporary abutment cap 80, which is most similar to the temporary abutment cap 480; however, the temporary abutment cap 480 has a different overall shape and/or size to correspond with the temporary abutment 410. Specifically, while the temporary abutment cap 480 includes one or more projections 486 (similar to the projections 86 of the temporary abutment cap 80 in FIG. 4A), the projections 486 (FIG. 8D) are formed by a continuous projection that circumscribes an inner surface 482 of the temporary abutment cap 480 that is separated into the projections 486 by a plurality of notches 487. The notches 487 allow for the temporary abutment cap 480 to be removed from the temporary abutment 410, when engaged in the snap-fit type engagement shown in FIG. 8F, with relatively less force than if the projections 486 were continuous (e.g., not separated by the notches 487). Alter-



15

natively, the projections **486** (FIG. **8D**) of the temporary abutment cap **480** can be formed in the same, or similar manner as the projections **86** (FIG. **4A**) of the temporary abutment cap **80** (e.g., without the notches **487**).

Additionally, the projections **486** (FIG. **8D**) are positioned 5 completely below the non-rotational structure **484** of the temporary abutment cap **480** as compared to the positioning of the projections **86** (FIG. **4A**) of the temporary abutment cap **80** which are positioned adjacent to a central region of the non-rotational structure **84** of the temporary abutment 10 cap **80** (e.g., the projections **86** of the temporary abutment cap **80** are relatively higher). The positioning of the projections **486** (FIG. **8D**) can aid in providing a seal between a lower or apical end (e.g., a bottom end **488**) of the temporary abutment cap **486** and the temporary abutment **410** (e.g., by 15 forcing the lower end downwardly). Irrespective of the placement of the projections **486** on the inner surface **482** of the temporary abutment cap **480**, the projections **486** (FIG. **8D**) function in the same, or similar, manner as the projections **86** (FIG. **4A**) in that the projections **486** (FIG. **8D**) are configured to mate with the continuous retention groove **432** of the temporary abutment **410** (FIG. **8B**) in a snap-fit type engagement (best shown in FIG. **8F**).

A further difference between the temporary abutment cap **480** (FIG. **8D**) and the temporary abutment cap **80** (FIG. **4A**) 25 is that the temporary abutment cap **480** includes an aperture **483** in a top portion thereof to provide access for the screw **470** to be installed after the temporary abutment cap **480** is installed on (e.g., snapped onto) the temporary abutment **410**. As described above in reference to the screw **470** of FIG. **8C**, the wall of the aperture **483** can engage with the lip **477** of the screw **470** for additional rigidity of the prosthesis assembly **400**.

Referring to FIGS. **8E** and **8F**, a cross-sectional exploded view (FIG. **8E**) and a cross-sectional assembled view (FIG. **8F**) of the prosthesis assembly **400** and the dental implant 35 **120** are shown for illustrating how the various components of the prosthesis assembly **400** are assembled and attached to the dental implant **120**. The dental implant **120** is installed in a patient's jawbone (not shown) and then the temporary abutment **410** is non-rotationally attached to the implant **120** via a non-rotational feature **422** (FIG. **8B**) and the screw **470**. The temporary abutment cap **480** is snap-fitted onto the temporary abutment **410** in a non-rotational manner such that the non-rotational structure **434** (FIG. **8B**) of the temporary abutment **410** engages the non-rotational structure **484** (FIG. **8D**) of the temporary abutment cap **480**. The temporary prosthesis **490** is coupled to the temporary abutment cap **480** in the same, or similar, manner as described herein in reference to the temporary prosthesis **90** being 45 coupled to the temporary abutment **80** (FIGS. **6A** and **6B**). Alternatively, as the temporary abutment cap **480** includes the aperture **483** (FIG. **8D**), the temporary abutment cap **480** can be snap-fitted onto the temporary abutment **410** prior to the screw **470** being installed. Then, the screw **470** can be 50 installed through the aperture **483**, which is followed by the temporary prosthesis **490** being coupled to the temporary abutment cap **480**.

Referring to FIGS. **9A** to **9E**, various views of components of an alternative prosthesis assembly **500** and the dental implant **120** are shown. As shown in FIG. **9A**, the prosthesis assembly **500** includes a temporary abutment **510**, a temporary abutment cap **580**, a screw **570**, and a temporary prosthesis **590**, each of which is similar to, or the same as, corresponding components of the previously described prosthesis assemblies. In FIGS. **9A** to **9E**, each of the components and features is identified by a **500-series** reference 60 numeral, and those **500-series** reference numerals correspond to like features of the various components and features of the previously described prosthesis assemblies. For example, reference numeral **534** is used to describe the non-rotational structure **534** (FIG. **9B**), which is the same as, or similar to, the non-rotational structure **34** (FIG. **1A**) and the non-rotational structure **434** (FIG. **8B**). Additionally, reference numerals **520**, **540**, **555**, **560**, **581**, and **587** are used in the figures to illustrate features that are the same as, or similar to, previously described features with reference numbers **20**, **40**, **55**, **60**, **81**, and **487** respectively.

Referring to FIG. **9B**, the temporary abutment **510** generally includes all of the same features as the temporary abutments **10** and **410**; however, several differences exist between the temporary abutment **510** and the temporary abutment **410**, which is most similar to the temporary abutment **510**. Specifically, the temporary abutment **510** includes a continuous retention groove **532** (FIG. **9B**) that is positioned directly above a flange **550** as compared to the positioning of the continuous retention groove **432** of the temporary abutment **410** (best shown by comparing FIG. **8E** with **9D**). Irrespective of the placement of the continuous retention groove **532** on a supragingival region **530** of the temporary abutment **510**, the continuous retention groove **532** (FIG. **9B**) functions in the same, or similar, manner as the continuous retention groove **432** (FIG. **8B**) in that the continuous retention groove **532** is configured to mate with one or more projections **586** of the temporary abutment cap **580** (FIG. **9C**) in a snap-fit type engagement (shown in FIG. **9E**).

A non-rotational structure **534** of the temporary abutment **510** is a six-sided hexagonal boss as compared to the single flat surface of the non-rotational structures **34**, **434** (see e.g., FIGS. **1A** and **8B**). Various other non-rotational structures can be used to prevent relative rotation between the temporary abutment **510** and the temporary abutment cap **580** (e.g., three-sided polygonal boss, four-sided polygonal boss, clover boss, etc.).

A further difference between the temporary abutment **510** (FIG. **9B**) and the temporary abutment **410** (FIG. **8B**) is that the temporary abutment **510** includes two informational marker locations **562** and one informational marker **564** as compared to the three informational marker locations **462** and the two informational marker **464** of the temporary abutment **410**. Moreover, the informational marker locations **562** of the temporary abutment **510** are in the shape of a rectangular surface and a triangular surface. The differently shaped informational marker locations **562** themselves can aid in providing information about the temporary abutment **510** and/or the underlying dental implant **120**. For example, a sole triangular informational marker location **562** can indicate a particular manufacturer and, for another example, both a rectangular and a triangular informational marker **562** on a temporary abutment can indicate a different manufacturer. 55

Referring to FIG. **9C**, the temporary abutment cap **580** generally includes all of the same features as the temporary abutment caps **80** and **480** except for a few differences. One or more projections **586** of the temporary abutment cap **580** are positioned relatively lower as compared to the positioning of the projections **486** of the temporary abutment cap **480** (best shown by comparing FIG. **8F** with FIG. **9E**). Irrespective of the placement of the projections **586** on an inner surface **582** of the temporary abutment cap **580**, the projections **586** (FIG. **9C**) function in the same, or similar, manner as the projections **86** (FIG. **4A**) in that the projections **586** (FIG. **9C**) are configured to mate with the con-



tinuous retention groove **532** of the temporary abutment **510** in a snap-fit type engagement (best shown in FIG. 9E).

A further difference between the temporary abutment cap **580** (FIG. 9C) and the temporary abutment cap **480** (FIG. 8D) is that the temporary abutment cap **580** includes a non-rotational structure **584** that is a six-sided hexagonal socket (FIG. 9C) as compared to the single flat surface of the non-rotational structure **484** of the temporary abutment cap **480** (FIG. 8D). The non-rotational structure **584** can be any of a variety of structures that corresponds with the non-rotational structure **534** to prevent relative rotation between the temporary abutment **510** and the temporary abutment cap **580**.

Referring to FIGS. 9D and 9E, a cross-sectional exploded view (FIG. 9D) and a cross-sectional assembled view (FIG. 9E) of the prosthesis assembly **500** and the dental implant **120** are shown for illustrating how the various components of the prosthesis assembly **500** are assembled and attached to the dental implant **120**. The dental implant **120** is installed in a patient's jawbone (not shown) and then the temporary abutment **510** is non-rotationally attached to the implant **120** via the non-rotational feature **522** (FIG. 9B) and the screw **570**. The temporary abutment cap **580** is snap-fitted onto the temporary abutment **510** in a non-rotational manner such that the non-rotational structure **534** (FIG. 9B) of the temporary abutment **510** engages the non-rotational structure **584** (FIG. 9C) of the temporary abutment cap **580**. The temporary prosthesis **590** is coupled to the temporary abutment cap **580** in the same, or similar, manner as described herein in reference to the temporary prosthesis **90** being coupled to the temporary abutment **80** (FIGS. 6A and 6B). Alternatively, as the temporary abutment cap **580** includes an aperture **583** (FIG. 9C), the temporary abutment cap **580** can be snap-fitted onto the temporary abutment **510** prior to the screw **570** being installed. Then, the screw **570** can be installed through the aperture **583**, which is followed by the temporary prosthesis **590** being coupled to the temporary abutment cap **580**.

Referring to FIGS. 10A to 10E, various views of components of an alternative prosthesis assembly **600** and the dental implant **120** are shown. As shown in FIG. 10A, the prosthesis assembly **600** includes a temporary abutment **610**, a temporary abutment cap **680**, and a screw **670**, each of which is similar to, or the same as, corresponding components of the previously described prosthesis assemblies. In FIGS. 10A to 10E, each of the components and features is identified by a **600-series** reference numeral, and those **600-series** reference numerals correspond to like features of the various components and features of the previously described prosthesis assemblies. For example, reference numeral **634** is used to describe the non-rotational structure **634** (FIG. 10B), which is the same as, or similar to, the non-rotational structure **34** (FIG. 1A).

Referring to FIG. 10B, the temporary abutment **610** generally includes most of the same features as the temporary abutments **10**, **410**, **510**; however, several differences exist between the temporary abutment **610** and the temporary abutment **510**, which is most similar to the temporary abutment **610**. Specifically, an outer surface **655** of a flange **650** of the temporary abutment **610** (e.g., the portion of the temporary abutment **610** between a subgingival region **620** and a supragingival region **630**) is relatively shorter as compared to the previous embodiments. A longer flange with an outer surface **655** having a relatively longer contour is not provided by the temporary abutment **610** as the shaping of contour of the patient's gingiva during healing is based mostly on the outer contours of the lower portion of

the temporary abutment cap **680**, the contours of which are best seen in FIG. 10E. Various other contours of the lower portion of the temporary abutment **680** can be used depending on the particular conditions present in the patient's mouth.

The temporary abutment **610** lacks the continuous retention groove **532** of the temporary abutment **510** as the temporary abutment cap **680** does not engage the temporary abutment **610** in a snap-fit type engagement. Rather, the temporary abutment cap **680** is coupled to the implant **120** and the temporary abutment **610** via the screw **670** as best shown in FIG. 10E.

A further difference between the temporary abutment **610** (FIG. 10B) and the temporary abutment **510** (FIG. 9B) is that the temporary abutment **610** includes one informational marker location **662** with two informational markers **664** thereon as compared to the two informational marker locations **562** and the one informational marker **564** of the temporary abutment **510**. The multiple informational markers **664** on the single informational marker location **662** results in the need for less informational marker locations **662**, which, depending on the size of the temporary abutment **610**, can be beneficial as the available real estate on a top surface **660** of the temporary abutment **610** is minimal due to, for example, an internal bore **640** of the temporary abutment **610**.

Referring to FIG. 10C, unlike the single-piece temporary abutment caps **80**, **280**, **480**, and **580**, the temporary abutment cap **680** includes two pieces—a customizable portion **680a** and a rigid portion **680b** (best seen when separated in FIGS. 10A and 10D). The customizable portion **680a** is similar to the additional material **282** of the temporary abutment cap **280** described above in reference to FIGS. 7A and 7B. That is, the customizable portion **680a** can be sculpted into a custom shape for a particular patient and/or come preformed having an anatomical tooth shape. The rigid portion **680b** is generally made from metal, such as, for example, titanium, and includes a non-rotational structure **684** and an internal bore **641**. Alternatively, the rigid portion **680b** can be made from a rigid plastic. The customizable portion **680a** is permanently attached to the rigid portion **680b**. However, in an alternative implementation, a kit of customizable portions **680a** can be packaged with one or more rigid portions **680b** such that a clinician selects one of the customizable portions **680a** and then permanently attaches the selected one with a selected rigid portion **680b** for attachment to the temporary abutment **610**.

The temporary abutment cap **680** lacks a snap-fit type engagement to the temporary abutment **610**. Rather, the temporary abutment cap **680** is coupled to the implant **120** and the temporary abutment **610** via the screw **670** as best shown in FIG. 10E.

The temporary abutment cap **680** includes the non-rotational structure **684** that is a six-sided hexagonal socket (FIG. 10C) as compared to the single flat surface of the non-rotational structure **84** of the temporary abutment cap **80** (FIG. 4A). However, the non-rotational structure **684** can be any of a variety of structures that corresponds with the non-rotational structure **634** to prevent relative rotation between the temporary abutment **610** and the temporary abutment cap **680**.

Similar to the temporary abutment **580** (FIG. 9C), the temporary abutment cap **680** includes an aperture **683** (FIG. 10E) in a top portion thereof to provide access for the screw **670** to be installed after the temporary abutment cap **680** is installed on (e.g., non-rotationally mounted on) the temporary abutment **610**. As best shown in FIG. 10E, a lip **677** of



the screw **670** engages with an internal shoulder **642** of the internal bore **641** of the temporary abutment cap **680** to hold the prosthesis assembly **600** on the implant **120**. After installation of the screw **670**, a plug (not shown) of like material to the customizable portion **680a** (e.g., plastic, acrylic, etc.) can be inserted through the aperture **683** and above the lip **677** of the screw **670** into the internal bore **641** to seal the aperture **683**.

Referring to FIGS. **10D** and **10E**, a cross-sectional exploded view (FIG. **10D**) and a cross-sectional assembled view (FIG. **10E**) of the prosthesis assembly **600** and the dental implant **120** are shown for illustrating how the various components of the prosthesis assembly **600** are assembled and attached to the dental implant **120**. The dental implant **120** is installed in a patient's jawbone (not shown) and then the temporary abutment **610** is non-rotationally attached to the implant **120** via a non-rotational feature **622** (FIG. **10B**). The two-piece temporary abutment cap **680** is non-rotationally coupled to the temporary abutment **610** such that the non-rotational structure **634** (FIG. **10B**) of the temporary abutment **610** engages the non-rotational structure **684** (FIG. **10C**) of the temporary abutment cap **680**. The screw **670** is then installed through the aperture **683** to hold the prosthesis assembly **600** on the implant **120**.

Referring to FIGS. **11A** to **11E**, various views of components of an alternative prosthesis assembly **700** and the dental implant **120** are shown. As shown in FIG. **11A**, the prosthesis assembly **700** includes a temporary abutment **710**, a screw **770**, a temporary abutment cap **780**, and a temporary prosthesis **790**, each of which is similar to, or the same as, corresponding components of the previously described prosthesis assemblies. In FIGS. **11A** to **11E**, each of the components and features is identified by a **700-series** reference numeral, and those **700-series** reference numerals correspond to like features of the various components and features of the previously described prosthesis assemblies. For example, reference numeral **734** is used to describe the non-rotational structure **734** (FIG. **11B**), which is the same as, or similar to, the non-rotational structure **34** (FIG. **1A**) and the non-rotational structure **534** (FIG. **9B**). Additionally, reference numerals **720**, **730**, **740**, **750**, **755**, **760**, **781**, **782**, **787**, and **788** are used in the figures to illustrate features that are the same as, or similar to, previously described features with reference numbers **20**, **30**, **40**, **50**, **55**, **60**, **81**, **82**, **487**, and **88**, respectively.

Referring to FIG. **11B**, the temporary abutment **710** generally includes all of the same features as the previous temporary abutments **10**, **410**, **510**, **610**, but lacks the informational marker locations **562** and the informational markers **564** of the temporary abutment **510**. Rather, the temporary abutment cap **780** (FIG. **11C**) of the prosthesis system **700** includes informational marker locations **762** and informational markers **764**.

Further, a continuous retention groove **732** (FIG. **11B**) of the temporary abutment **710** is positioned relatively higher (e.g., relatively further from the flange **50**) as compared to the positioning of the continuous retention groove **532** of the temporary abutment **510** (best shown by comparing FIG. **9D** with **11D**). The continuous retention groove **732** (FIG. **11B**) functions in the same, or similar, manner as the continuous retention grooves previously described herein in that the continuous retention groove **732** is configured to mate with one or more projections **786** of the temporary abutment cap **780** (FIG. **11C**) in a snap-fit type engagement (shown in FIG. **11E**).

Referring to FIG. **11C**, the temporary abutment cap **780** includes the informational marker locations **762** and the

informational markers **764**. The information indicated by the informational marker locations **762** and/or the informational markers **764** (e.g., location and orientation of the underlying implant **120**) can be gathered by scanning the temporary abutment cap **780** as opposed to scanning the temporary abutment **710**.

Further, the temporary abutment cap **780** lacks the aperture **583** of the temporary abutment cap **580** in a similar fashion to the temporary abutment cap **80** lacking the aperture **583**. Alternatively, the temporary abutment cap **780** can include an aperture (not shown) similar to the aperture **583** of the temporary abutment cap **580**.

Referring to FIGS. **11D** and **11E**, a cross-sectional exploded view (FIG. **11D**) and a cross-sectional assembled view (FIG. **11E**) of the prosthesis assembly **700** and the dental implant **120** are shown for illustrating how the various components of the prosthesis assembly **700** are assembled and attached to the dental implant **120**. The dental implant **120** is installed in a patient's jawbone (not shown) and then the temporary abutment **710** is non-rotationally attached to the implant **120** via a non-rotational feature **722** (FIG. **11B**) and the screw **770**. The temporary abutment cap **780** is snap-fitted onto the temporary abutment **710** in a non-rotational manner such that the non-rotational structure **734** (FIG. **11B**) of the temporary abutment **710** engages a non-rotational structure **784** (FIG. **11C**) of the temporary abutment cap **780**.

Optionally, a temporary prosthesis **790** can be coupled to the temporary abutment cap **780** in the same, or similar, manner as described herein in reference to the temporary prosthesis **90** being coupled to the temporary abutment **80** (FIGS. **6A** and **6B**). In such an alternative implementation, the informational marker locations **762** and/or the informational markers **764** can also mate with correspondingly shaped internal surfaces (not shown) of the temporary prosthesis **790** to provide for anti-rotation between the temporary abutment cap **780** and the temporary prosthesis **790**. In the case that the temporary prosthesis **790** is not coupled to the temporary abutment cap **780**, the temporary abutment cap **780** itself can have an anatomically shaped tooth structure and act as a temporary prosthesis.

Referring to FIGS. **12A** to **12E**, various views of components of an alternative prosthesis assembly **800** and the dental implant **120** are shown. As shown in FIG. **12A**, the prosthesis assembly **800** includes a temporary abutment **810**, a temporary abutment cap **880**, a screw **870**, and a temporary prosthesis **890**, each of which is similar to, or the same as, corresponding components of the previously described prosthesis assemblies. In FIGS. **12A** to **12E**, each of the components and features is identified by a **800-series** reference numeral, and those **800-series** reference numerals correspond to like features of the various components and features of the previously described prosthesis assemblies. For example, reference numeral **834** is used to describe the non-rotational structure **834** (FIG. **12B**), which is the same as, or similar to, the non-rotational structure **34** (FIG. **1A**) and the non-rotational structure **534** (FIG. **9B**). Additionally, reference numerals **820**, **830**, **850**, **855**, **860**, **881**, and **888** are used in the figures to illustrate features that are the same as, or similar to, previously described features with reference numbers **20**, **30**, **50**, **55**, **60**, **81**, and **88**, respectively.

Referring to FIG. **12B**, the temporary abutment **810** generally includes all of the same features as the temporary abutments of the previous embodiments except the temporary abutment **810** lacks the continuous retention groove **732** (FIG. **11B**) of the temporary abutment **710** such that the temporary abutment **810** does not couple with the temporary



## 21

abutment cap **880** (FIG. 12C) in a snap-fit type engagement. Rather, the temporary abutment cap **880** (FIG. 12C) is held in a non-rotational fashion onto the temporary abutment **810** (FIG. 12B) via the screw **870**, which is best shown in FIG. 12E. Accordingly, the temporary abutment cap **880** lacks the one or more projections **786** (FIG. 11C) of the temporary abutment cap **780** such that the temporary abutment cap **880** (FIG. 12C) does not couple with the temporary abutment **810** in a snap-fit type engagement.

Additionally, the temporary abutment cap **880** includes an aperture **883** that is similar to the aperture **583** of the temporary abutment cap **580** (FIG. 9C). The aperture **883** provides a path for the screw **870** to mate with the implant **120** through the internal bore **840** of the temporary abutment **810**, thereby securing the temporary abutment cap **880** and the temporary abutment **810** onto the implant **120** in a non-rotational fashion, as best shown in FIG. 12E. The screw **870** (FIG. 12A) has a different head as compared to the screw **770**. The head of the screw **870** includes a groove for mating with an O-ring **873** (FIG. 12E) that aids in sealing the internal bore **840** (FIG. 12B) of the temporary abutment **810**.

Referring to FIGS. 12D and 12E, a cross-sectional exploded view (FIG. 12D) and a cross-sectional assembled view (FIG. 12E) of the prosthesis assembly **800** and the dental implant **120** are shown for illustrating how the various components of the prosthesis assembly **800** are assembled and attached to the dental implant **120**. The dental implant **120** is installed in a patient's jawbone (not shown) and then the temporary abutment **810** is non-rotationally attached to the implant **120** via a non-rotational feature **822** (FIG. 12B). The temporary abutment cap **880** is coupled to the temporary abutment **810** in a non-rotational manner such that the non-rotational structure **834** (FIG. 12B) of the temporary abutment **810** engages a non-rotational structure **884** (FIG. 12C) of the temporary abutment cap **880**. The screw **870** is inserted through the aperture **883** of the temporary abutment cap **880** and the internal bore **840** of the temporary abutment **810** and is threadingly coupled to the implant **120**.

Optionally, a temporary prosthesis **890** is coupled to the temporary abutment cap **880** in the same, or similar, manner as described herein in reference to the temporary prosthesis **90** being coupled to the temporary abutment **80** (FIGS. 6A and 6B). In such an alternative implementation, the informational marker locations **862** and/or the informational markers **864** can also mate with correspondingly shaped internal surfaces (not shown) of the temporary prosthesis **890** to provide for anti-rotation between the temporary abutment cap **880** and the temporary prosthesis **890**. In the case that the temporary prosthesis **890** is not coupled to the temporary abutment cap **880**, the temporary abutment cap **880** itself can have an anatomically shaped tooth structure and act as a temporary prosthesis.

Referring to FIGS. 13A to 13H, various views of components of an alternative prosthesis assembly **900** and the dental implant **120** are shown. As shown in FIG. 13A, the prosthesis assembly **900** includes a temporary abutment **910**, a temporary abutment cap **980**, a screw **970**, and a temporary prosthesis **990**, each of which is similar to, or the same as, corresponding components of the previously described prosthesis assemblies. In FIGS. 13A to 13H, each of the components and features is identified by a **900**-series reference numeral, and those **900**-series reference numerals correspond to like features of the various components and features of the previously described prosthesis assemblies. For example, reference numeral **934** is used to describe the

## 22

non-rotational structure **934** (FIGS. 13B and 13C), which is the same as, or similar to, the non-rotational structure **34** (FIG. 1A) and the non-rotational structure **534** (FIG. 9B). Additionally, reference numerals **932**, **960**, **962**, **982**, **986**, **987**, and **988** are used in the figures to illustrate features that are the same as, or similar to, previously described features with reference numbers **432**, **60**, **62**, **82**, **486**, **487**, and **88**, respectively.

Referring to FIGS. 13B and 13C, the temporary abutment **910** generally includes all of the same features as the temporary abutments of the previous embodiments except an outer surface **955** of a flange **950** (e.g., portion of **910** that separates a subgingival region **920** and a supragingival region **930**) of the temporary abutment **910** has a differently shaped contour for mating with a bottom end **988** (FIGS. 13D and 13E) of the temporary abutment cap **980**. Rather than the bottom end **988** resting on a substantially flat upper portion of the flange **950** (as the bottom end **588** of the temporary abutment cap **580** rests on the upper portion of the flange **50** shown in FIG. 9E), the bottom end **988** abuts the flange **950** and forms a portion of the contour (best shown in FIG. 13G) that aids in forming a patient's gingival tissue during the healing process. Various other contours of the bottom end **988** and of the outer surface of the flange **950** can be used depending on the particular conditions present in the patient's mouth.

The temporary abutment **910** includes internal capture threads **943** (FIG. 13C) for threadably engaging with and capturing the screw **970**. Such threads **943** are particularly useful for temporarily coupling the temporary abutment **910** with the screw **970** prior to installation of the same in a patient's mouth. As the screw **970** is rather small in size, its manipulation can be difficult. Thus, the temporary coupling between the screw **970** and the temporary abutment **910** prior to being installed in the patient's mouth prevents a clinician from having to perform the potentially difficult step of separately placing the screw **970** within an internal bore **940** for attachment with the implant **120** after the temporary abutment **910** is installed in the patient's mouth. While the threads **943** are only shown and described as being included in the temporary abutment **910**, the same, or similar, threads can be included in any of the other temporary abutments of the present disclosure.

Referring to FIGS. 13D and 13E, a generally cylindrical outer surface **981** of the temporary abutment cap **980** includes a plurality of grooves, notches, ribs, knurling, etc., or any combination thereof, instead of a substantially smooth generally cylindrical outer surface **581** (FIG. 9C) of the temporary abutment cap **580**. The generally cylindrical outer surface **981** provides relatively more surface area as compared to the smooth generally cylindrical outer surface **581**. The additional surface area of the generally cylindrical outer surface **981** results in a better adhesion or attachment between the temporary abutment cap **980** and the temporary prosthesis **990** (shown in FIGS. 13G and 13H). Alternatively to an inner bore of the temporary prosthesis **990** being formed to correspond to the contours of the generally cylindrical outer surface **981** of the temporary abutment cap **980** (best shown in FIGS. 13A and 13F), the temporary prosthesis **990** can be sufficiently pliable such that the inner bore of the temporary prosthesis **990** can be formed with one of a variety of shapes (e.g., substantially cylindrical and smooth) and slid over the temporary abutment cap **980**.

Referring to FIGS. 13F to 13H, a cross-sectional exploded view (FIG. 13F), a cross-sectional assembled view (FIG. 13G), and a partial front and partial cross-sectional assembled view (FIG. 13H) of the prosthesis assembly **900**



and the dental implant **120** are shown for illustrating how the various components of the prosthesis assembly **900** are assembled and attached to the dental implant **120**. The dental implant **120** is installed in a patient's jawbone (not shown) and then the temporary abutment **910** is non-rotationally attached to the implant **120** via a non-rotational feature **922** (FIGS. **13B** and **13C**) and the screw **970**. The temporary abutment cap **980** is snap-fitted onto the temporary abutment **910** in a non-rotational manner such that the non-rotational structure **934** (FIGS. **13B** and **13C**) of the temporary abutment **910** engages a non-rotational structure **984** (FIGS. **13D** and **13E**) of the temporary abutment cap **980**. The temporary prosthesis **990** is coupled to the temporary abutment cap **980** in the same, or similar, manner as described herein in reference to the temporary prosthesis **90** being coupled to the temporary abutment **80** (FIGS. **6A** and **6B**) and such that the generally cylindrical outer surface **981** (FIGS. **13D** and **13E**) engages the internal bore of the temporary prosthesis **990**. Alternatively, as the temporary abutment cap **980** includes an aperture **983** (FIGS. **13D** and **13E**), the temporary abutment cap **980** can be snap-fitted onto the temporary abutment **910** prior to the screw **970** being installed. Then, the screw **970** can be installed through the aperture **983**, which is followed by the temporary prosthesis **990** being coupled to the temporary abutment cap **980**.

Referring to FIGS. **14A-C**, three exploded prosthesis assemblies **1000a** (FIG. **14A**), **1000b** (FIG. **14B**), and **1000c** (FIG. **14C**) are shown for connection with three different dental implants **120** (FIG. **14A**), **121a** (FIG. **14B**), and **121b** (FIG. **14C**), where like reference numbers are used for like components previously described herein. Each of the implants **120**, **121a**, and **121b** includes a different anti-rotational feature for non-rotationally mating with a corresponding anti-rotational feature of a temporary abutment. As shown, the first implant **120** includes a female or socket-type hexagonal anti-rotational feature **120'**, the second implant **121a** includes a male or boss-type hexagonal anti-rotational feature **121a'**, and the third implant **121b** includes a male star anti-rotational feature **121b'**. Various other types and shapes of anti-rotational features are contemplated for non-rotationally mating with corresponding anti-rotational features of a temporary abutment (e.g., temporary abutments **910**, **911a**, and **911b**).

Each of the prosthesis assemblies **1000a**, **1000b**, and **1000c** includes an identical temporary prosthesis **990**, an identical screw **970**, and an identical temporary abutment cap **980**. However, while the temporary abutments **910**, **911a**, and **911b** of each of the prosthesis assemblies **1000a**, **1000b**, and **1000c** have identical external supragingival regions **930** and flanges **950**, the subgingival regions **920**, **921a**, and **921b**, and the internal arrangements of each of the temporary abutments **910**, **921a**, and **921b** are different for non-rotationally mating with the different anti-rotational features **120'**, **121a'**, and **121b'** of the implants **120**, **121a**, and **121b**, respectively. Thus, depending on the type and/or manufacturer of the underlying implant, a temporary abutment (e.g., temporary abutments **910**, **911a**, **911b**) can be selected (e.g., from a kit of temporary abutments) having a corresponding subgingival region (e.g., subgingival region **920**, **921a**, **921b**) that non-rotationally couples therewith, but also includes a standard external supragingival region **930** and flange **950** that is configured to be coupled with standard components thereafter (e.g., the temporary prosthesis **990**, the screw **970**, and the temporary abutment cap **980**).

While the supragingival regions **930** and the flanges **950** of the implants **120**, **121a**, and **121b** are described as being

identical, the number and/or orientation of the informational markers **964** and/or the informational marker locations **962** can be different. For example, as shown in FIG. **14A**, the first temporary abutment **910** includes an informational marker location **962** with a single informational marker **964** thereon, which can, for example, indicate that the underlying implant **120** includes a female/socket-type hexagonal anti-rotational feature **120'**. Similarly, as shown in FIG. **14B**, the second temporary abutment **911a** includes an informational marker location **962** with two informational markers **964** thereon, which can, for example, indicate that the underlying implant **121a** includes a male/boss-type hexagonal anti-rotational feature **121a'** and, as shown in FIG. **14C**, the third temporary abutment **911b** includes an informational marker location **962** with three informational markers **964** thereon, which can, for example, indicate that the underlying implant **121b** includes a male/boss-type star anti-rotational feature **121b'**. The differences in the informational markers **964** of the three temporary abutments **910**, **911a**, and **911b** may alternatively and/or additionally indicate a different line of implants for a single manufacturer, or a different line of different implant manufacturers. Of course, additional informational markers **964** and/or additional informational marker locations **962** on the temporary abutments **910**, **911a**, and **911b** could indicate other aspects of the underlying implants **120**, **121a**, and **121b** (e.g., diameter, anti-rotational feature orientation, location of the table surface, etc.).

While some of the anti-rotational features are shown in the figures and described herein as being a male or boss anti-rotational feature and others are shown in the figures and described herein as being female or socket anti-rotational features, it is contemplated that the male-female anti-rotation features can be swapped on different components as needed.

While the temporary abutments **10**, **10'**, **410**, **510**, **610**, **710**, **810**, and **910** are shown and described herein as being temporary (i.e., not permanent), the temporary abutments **10**, **10'**, **410**, **510**, **610**, **710**, **810**, and **910** can, in fact, be permanent abutments that are designed to be coupled with a corresponding permanent prosthesis and/or crown. In such an alternative implementation of the disclosed concepts, the permanent prosthesis is developed and designed to be coupled with the temporary abutment **10**, **10'**, **410**, **510**, **610**, **710**, **810**, and **910** instead of a separate permanent patient specific abutment.

While the temporary abutments **10**, **10'**, **410**, **510**, **610**, **710**, **810**, and **910** are shown and described herein as having a subgingival region, a supragingival region and a flange therebetween, any portion of the flange and/or of the supragingival region can be placed subgingival (e.g., below the gingival tissue) for a given installation. Similarly, any portion of the flange and/or of the subgingival region can be placed supragingival (e.g., above the gingival tissue) for a given installation. Moreover, the supragingival regions described herein can be referred to as a post region that is partially subgingival and/or partially supragingival. That is, in some instances, the terms supragingival and post can be used interchangeably when referring to the various portions of the temporary abutments described herein.

All of the temporary prostheses **90**, **490**, **590**, **790**, **890**, and **990** described herein can be cemented to the respective temporary abutment caps **80**, **480**, **580**, **780**, **880**, and **980** described herein via normal dental cement.

In the various embodiments of FIGS. **1A** to **14C**, the temporary abutments, the temporary abutment caps, and the temporary prostheses have several physical and functional differences. However, each embodiment is useful in that it



25

provides an aesthetically pleasing temporary prosthesis that can be installed immediately after implant installation and that can be used to form the adjacent gingival tissue into a desired shape as it heals following surgery. Additionally, the temporary abutment caps and temporary prostheses (which are typically held together via dental cement) can be easily removed from the temporary abutment to reveal the informational markers thereon that provide information about the dimensions and/or orientation of the underlying implant and/or of the temporary abutment itself (or the temporary abutment cap may include the information markers such that removal is not required). Knowing this information regarding the dimensions and/or orientation of the underlying implant and/or the temporary abutment and knowing the actual healed shape of the gingival tissue (or a predicted healed shape, see FIG. 17 below) permits for the design and manufacture of a permanent patient-specific abutment prior to the patient's gingival tissue healing. It also provides for the option of the design and manufacture of the final permanent prosthesis that will fit on the patient-specific abutment.

Regarding one exemplary use of the informational markers disclosed herein (e.g., informational markers 64), an implant line may come in two diameters at the upper table surface (e.g., 4 mm and 5 mm). For each of those two implants, there may be four different types of temporary abutments that can be used. For example, there could be two different overall heights to the temporary abutment (e.g., 8 mm, and 10 mm). And, for each of those two temporary abutments having different heights, there could be two different emergence profiles (e.g., outer surface 55) leading away from the implant to the flange (e.g., flange 50) of the temporary abutment. As such, there are eight potential temporary abutments with different shapes and dimensions. If there are three informational marker locations (e.g., informational marker locations 62) on each of those temporary abutments at which an informational marker may or may not be present, that provides for eight combinations, assuming a binary-type marking system is used. Hence, each of the eight potential temporary abutments would have a unique marking scheme such that the exact temporary abutment can be easily identified by simple inspection (e.g., via scanning) of the informational markers. And, by knowing the exact temporary abutment, important information concerning the implant, such as its table's diameter (i.e., 4 mm or 5 mm) and the exact location of the implant's table (and its angular orientation), is also known. Additionally, by providing another informational marker (or a second type of informational marker location, such as a triangular or rectangular chamfer or flat) on the temporary abutment, the angular orientation of the implant's anti-rotational feature is known, which is also important for developing the permanent patient-specific abutment. In all of these embodiments, the computer system that receives and uses the scan data for developing the patient-specific abutment preferably includes a simple look-up table that, based on the information markers revealed in the scan, indicates the exact temporary abutment mounted on the implant. Then, the implant's information can be modeled in the computer system as well. This is, of course, one exemplary embodiment and more or less information markers may be needed depending on the type of implant system. As another example, the type of implant (e.g., its table's diameter and/or its type of anti-rotational connection) can be identified via informational markers present on the head of the screw that holds the temporary abutment to the implant. And, the informational markers on the temporary abutment indicate information

26

regarding the temporary abutment (e.g., its emergence profile shape, its overall height, its flange diameter, etc.).

#### Methods of Developing Permanent Patient-Specific Abutments and Tooth Prostheses

Referring to FIG. 15, a method (1100) of developing a permanent patient-specific abutment ("PSA") and tooth prosthesis typically begins with the installation (1102) of a dental implant (e.g., dental implant 120 shown in FIG. 6A) in the jawbone of a patient. A temporary abutment (e.g., temporary abutment 10, 10', 410, 510, 610, 710, 810, 910) is then installed (1104) in a non-rotational fashion on the implant directly after the implant is installed in the patient's jawbone. The temporary abutment is attached via complementary non-rotational features on the temporary abutment and on the implant. The temporary abutment is axially held in contact with the implant via a fastening device (e.g., fastening device 70, 470, 570, 670, 770, 870, 970) that threadably engages threads in an interior bore of the implant.

A temporary abutment cap (e.g., temporary abutment cap 80, 280, 480, 580, 680, 780, 880, 980) is attached (1106) to the temporary abutment in a removable fashion, such as, for example, via a snap-fit connection. Thereafter, or prior to the temporary abutment cap being attached, a temporary prosthesis, shaped to approximate an anatomically shaped tooth, is attached (1106) to the temporary abutment via the temporary abutment cap. The temporary prosthesis is generally affixed to the temporary abutment cap in a non-removable fashion (e.g., using acrylic, cement, bonding, etc.).

After the temporary components are installed (1104-1106), the patient's gingival tissue is permitted to heal therearound (1108). After the gingival tissue is healed, the temporary abutment cap and the temporary prosthesis are removed from the temporary abutment (1110). Removal of the temporary abutment cap and temporary prosthesis reveals a top surface of the underlying temporary abutment that includes one or more informational markers (e.g., informational markers 64). Additionally, an emergence profile of the healed gingival tissue is exposed, which may be in a non-round anatomical shape.

Both the temporary abutment and the surrounding gingival tissue are scanned using one or more scanning techniques directly in the patient's mouth (1112). Alternatively, an impression of at least the area of the patient's mouth including the temporary abutment is taken and scanned (1112). That is, the impression of the mouth can be scanned instead of scanning directly in the patient's mouth. In a third alternative, a physical model of the patient's dental conditions including the temporary abutment is made from the impression. Then the physical model can be scanned (1112) instead of scanning directly in the mouth or scanning the impression. In any event, scanning directly in the mouth is the preferred method.

Scan data is generated from the scanning that is analyzed via one or more processors and/or computers to obtain information (1114). Specifically, information related to and/or representative of the anatomically shaped emergence profile of the patient's gingival tissue surrounding the temporary abutment and information related to and/or representative of the informational markers on the temporary abutment (1114) is obtained. Additionally, information related to and/or representative of the patient's dental anatomy (e.g., adjacent teeth) surrounding the temporary abutment can be obtained. Further, information related to and/or representative of the geometrical relationships between the patient's



emergence profile, the informational markers, and/or the patient's dental anatomy can be obtained.

After the scanning, the temporary abutment cap and the temporary prosthesis are reattached to the temporary abutment (1116). A three-dimensional virtual model of at least a portion of the patient's mouth/dental conditions is created from the scan data (1118). The three-dimensional virtual model includes a virtual model of at least a portion of the patient's gingiva tissue, the patient's teeth, and the temporary abutment. Using one or more software or computer programs in conjunction with determined parameters based on the scanned informational markers, the three-dimensional virtual model can be modified to remove the temporary abutment, thereby providing/illustrating the location and orientation of the underlying implant and its relative position to the patient's gingival tissue. One non-limiting example is CAD-CAM dental software and scanning software available from 3Shape A/S located in Copenhagen, Denmark.

Using the three-dimensional model, a patient-specific abutment and permanent tooth prosthesis is virtually designed (1120). The designed patient-specific abutment and permanent tooth prosthesis can be created by, for example, sending data to a milling machine and/or a rapid prototype machine that is configured to create a physical patient-specific abutment (which would be attached to the implant) and a physical-permanent tooth prosthesis (which would be attached to the physical patient-specific abutment) that are both eventually installed in the mouth of the patient. After the patient-specific abutment and the permanent tooth prosthesis are created, the temporary abutment, the temporary abutment cap, and the temporary prosthesis are removed from the patient's mouth to expose the underlying dental implant (1122). The method is completed by installing the patient-specific abutment and the permanent tooth prosthesis on the dental implant as is known in the art (1124).

Prior to the dental implant being installed in the patient's mouth, several additional steps can be taken to aid in the installation process. Referring to FIG. 16, a method (1150) of creating and installing a patient-specific abutment and a permanent tooth prosthesis including preparation steps is shown. The preparation steps typically begin by scanning the patient's mouth to obtain initial scan data (1152). The scanning includes two types of scans to obtain data related to and/or representative of different types of tissues. A first soft tissue scan includes a scan configured to obtain data representative of soft tissue in the patient's mouth, such as, for example, the gingival tissue. A second hard tissue or bone scan includes a scan configured to obtain data representative of hard tissue or bone or teeth in the patient's mouth, such as, for example, the patient's jawbone and teeth. Additional details on creating accurate bone and soft-tissue digital dental models can be found in US Patent Application Publication No. 2011/0129792, entitled "Method of Creating an Accurate Bone and Soft-Tissue Digital Dental Model," which is hereby incorporated by reference herein in its entirety.

After obtaining the initial scan data, a three-dimensional model of the patient's mouth is created including the patient's bone structure and gingival tissue structure (1154). From the three-dimensional model, using one or more processors and/or computers, a desired location and orientation (e.g., pitch, yaw, depth) of a dental implant to be installed in the patient's mouth is determined (1156). The determined location can be selected or determined based on a number of different variables, such as, for example, the location, position, and orientation of the teeth adjacent to the proposed implant site, the location of nerves or the sinus

cavity, and/or the composition and structure of the patient's jawbone. Additional details on surgical guides and methods for using and making the same can be found in U.S. Patent Application Publication 2009/0130630, application Ser. No. 12/271,517, filed Nov. 14, 2008, entitled, "Components for Use with a Surgical Guide for Dental implant Replacement" and in U.S. Patent Application Publication 2009/0263764, application Ser. No. 12/425,202, filed Apr. 16, 2009, now allowed, entitled, "Method for Pre-Operative Visualization of Instrumentation Used with a Surgical Guide for Dental Implant Placement," each of which is hereby incorporated by reference in its entirety.

After the location is determined, a surgical template for installing the implant is created (1158). The surgical template is used to guide and/or aid a surgeon in drilling an aperture in the patient's mouth to receive the implant in the predetermined desired location. The preparation steps typically conclude with the positioning of the surgical guide in the patient's mouth prior to installation of the implant (1160). The rest of the steps directed to creating and installing the patient-specific abutment and the permanent tooth prosthesis (1102-1124) in the method (1150) are the same as previous described in reference to FIG. 15.

Referring to FIG. 17, an alternative method (1200) of developing a permanent patient-specific abutment ("PSA") and tooth prosthesis is described. A primary difference between the method (1200) and the methods (1100) and (1150) of FIGS. 15 and 16 is the timing of the scanning of the patient's mouth. As described below, in the method (1200), the patient's mouth is scanned at the same time that the implant is installed instead of waiting to permit gingival healing to occur prior to removing components and then scanning. Such a method (1200) can eliminate at least one visit to the doctor's office during the overall installation of the PSA and tooth prosthesis. More specifically, in some instances, the saved doctor's office visit prevents additional disruption of gingival tissue during the healing phase as the temporary abutment cap and temporary prosthesis do not have to be removed for scanning the patient's mouth a second time to capture the gingival contours.

The method (1200) typically begins with the installation (1202) of a dental implant (e.g., dental implant 120 shown in FIG. 6A) in the jawbone of a patient. A temporary abutment (e.g., temporary abutment 10, 10', 410, 510, 610, 710, 810, 910) is then installed (1204) in a non-rotational fashion on the implant directly after the implant is installed in the patient's jawbone. The temporary abutment is attached via complementary non-rotational features on the temporary abutment and on the implant. The temporary abutment is axially held in contact with the implant via a fastening device (e.g., screw 70, 470, 570, 670, 770, 870, and 970) that threadably engages threads in an interior bore of the implant.

After the attachment of the temporary abutment, a top surface thereof, that includes one or more informational markers (e.g., informational markers 64), is exposed in the patient's mouth. The temporary abutment and at least a portion of the surrounding dental features (e.g., adjacent teeth and/or adjacent gingival tissue) are scanned using one or more scanning techniques directly in the patient's mouth (1206). Alternatively, an impression of at least the area of the patient's mouth including the temporary abutment is taken and scanned (1206). That is, the impression of the mouth can be scanned instead of scanning directly in the patient's mouth. In a third alternative, a physical model of the patient's dental conditions including the temporary abutment is made from the impression. Then the physical model



can be scanned (1206) instead of scanning directly in the mouth or scanning the impression. In any event, scanning in the mouth is the preferred method.

A temporary prosthesis (e.g., temporary prosthesis 490, 590, 790, 890, 990), shaped to approximate an anatomically shaped tooth, is attached to a temporary abutment cap (e.g., temporary abutment cap 80, 280, 480, 580, 680, 780, 880, 980) outside of the patient's mouth (1208). The temporary prosthesis is generally affixed to the temporary abutment cap in a non-removable fashion (e.g., using acrylic, cement, bonding, etc.), thereby forming a subassembly; however, in some implementations of the present aspects, the temporary prosthesis is not permanently affixed to the temporary abutment cap until the temporary abutment cap is attached to the temporary abutment in the patient's mouth via a screw. Prior to and/or after attaching the temporary prosthesis to the temporary abutment cap, the temporary prosthesis can be shaped and/or customized (1210), by, for example, a clinician.

After the temporary prosthesis and the temporary abutment cap are attached and the final shape of the temporary prosthesis has been developed, the subassembly is scanned outside of the patient's mouth using one or more scanning techniques (1212). The subassembly (e.g., the temporary prosthesis and the temporary abutment cap) is then attached (1214) to the temporary abutment in a removable fashion, such as, for example, via a snap-fit connection and/or a screw-type connection. After the temporary components are installed (1214) and the scanning has taken place (1212), the patient's gingival tissue is permitted to heal therearound (1216).

Alternatively to scanning the subassembly outside of the patient's mouth, if the opening in the patient's gingiva is large enough—such that all the contours of the subassembly are viewable/scanable when attached to the temporary abutment—the scanning of the subassembly can occur in the mouth instead of outside the mouth. Such a scanning of the subassembly in the patient's mouth can occur immediately after installation and could include information representative of one or more surrounding features of the patient's mouth (e.g., adjacent teeth, gingival tissue, etc.).

Scan data is generated from both of the scans that is analyzed via one or more processors and/or computers to obtain information (1218 and 1220). The analysis of the scan data can occur immediately after the scans are taken and before the gingival tissue is permitted to heal. Of course, the analysis of the scan data can alternatively occur at any time after the gingival tissue is initially permitted to heal. Specifically, the first set of scan data is analyzed to obtain information related to and/or representative of the temporary abutment and information related to and/or representative of the informational markers on the temporary abutment (1218). Additionally, information related to and/or representative of the patient's dental anatomy (e.g., adjacent teeth) surrounding the temporary abutment can be obtained from the first set of scan data. Further, the second set of scan data is analyzed to obtain information related to and/or representative of the temporary prosthesis and/or the temporary abutment cap (1220). Specifically, information, such as, for example, the anatomical contours of the temporary prosthesis can be obtained. Such contours of the temporary prosthesis can be used to predict the contours of the patient's gingiva after being permitted to heal (1216).

After the scan data is acquired and analyzed, the first and the second sets of data are merged to create a three-dimensional virtual model of at least a portion of the patient's mouth/dental conditions (1222). The merging of

the data sets includes aligning the two data sets, which can be accomplished many ways. For example, corresponding markers (e.g., notches, grooves, lines, dots, pimple, dimple, etc.) positioned on, for example, a top side of the flange of the temporary abutment and on, for example, a bottom or under/inner surface of the temporary abutment cap can be captured during the scanning such that the markers can be used in conjunction with one or more software or computer programs to align (e.g., rotational align about the z-axis) the two sets of data with respect to each other. For another example, the two sets of data can be aligned using one or more software or computer programs that evaluate the positions of the non-rotational features of the temporary abutment and the temporary abutment cap. For a third example, the subassembly can be installed on the temporary abutment and a third scan is taken of the subassembly and surrounding area in the patient's mouth. The third scan produces a third set of scan data that can be used by one or more software or computer programs to align the first and the second data sets.

The three-dimensional virtual model includes a virtual model of at least a portion of the patient's gingiva tissue (based on one or both sets of the scan data), the patient's teeth, and the temporary abutment. Using one or more software or computer programs in conjunction with determined parameters based on the scanned informational markers, the three-dimensional virtual model can be modified to remove the temporary abutment, thereby providing/illustrating the location and orientation of the underlying implant and its relative position to the patient's gingival tissue. Further, using one or more software or computer programs, the three-dimensional virtual model is designed such that the depicted emergence profile of the patient's gingival tissue adjacent to the implantation site is based on the contours of the temporary prosthesis and/or the temporary abutment cap. That is, the depicted emergence profile in the three-dimensional virtual model is a predicted emergence profile and is not based on scan data from a scan of an actual (e.g., healed) emergence profile of the patient's gingival tissue because the scan in the mouth was taken prior to gingival healing.

Using the three-dimensional model, a patient-specific abutment and permanent tooth prosthesis is virtually designed (1224). The designed patient-specific abutment and permanent tooth prosthesis can be created by, for example, sending data to a milling machine and/or a rapid prototype machine that is configured to create a physical patient-specific abutment and/or a physical-permanent tooth prosthesis that are both eventually installed in the mouth of the patient. Alternatively and/or in addition thereto, one or more rapid prototype models of the patient's mouth, including a replica of the gingival contours, can be fabricated based on the three-dimensional model. The rapid prototype model(s) with the permanent tooth prosthesis thereon can be used by a clinician to develop, for example, the permanent prosthesis.

After the patient-specific abutment and the permanent tooth prosthesis are created, the temporary abutment, the temporary abutment cap, and the temporary prosthesis are removed from the patient's mouth to expose the underlying dental implant (1226). The method is completed by installing the patient-specific abutment and the permanent tooth prosthesis on the dental implant as is known in the art (1228).

In addition to the above described method (1200), after the gingival tissue is at least partially healed, if a clinician determines that the predicted emergence profile of the patient's gingival tissue is inaccurate due to, for example,



31

the tissue healing in an unpredicted manner or shape, modifications can be made to, for example, the three-dimensional model, the temporary prosthesis, the temporary abutment cap, etc. Specifically, the temporary prosthesis and the temporary abutment cap can be removed from the temporary abutment and the temporary prosthesis can be reshaped and/or modified to better shape the gingival tissue in preparation for installing the permanent components. In such an instance of physically modifying the temporary prosthesis after partial healing has occurred, the modified temporary prosthesis and temporary abutment cap is scanned to produce a third set of scan data. The third set of scan data can then be used in the same fashion as the second set of scan data was originally used. In essence, the third set replaces the second set and the three-dimensional virtual model is redesigned to include a newly predicted gingival emergence profile.

Alternatively, in the case that the clinician determines that the predicted emergence profile of the patient's gingival tissue is, for example, slightly inaccurate, but that physical modification of the temporary prosthesis is unnecessary, virtual manipulation of the three-dimensional virtual model can be made in lieu of physical modification such that the designed permanent components are based on a newly predicted gingival emergence profile that accounts for the slight inaccuracies of the original predicted profile.

While the illustrated embodiments have been primarily described with reference to the development of a patient-specific abutment for a single tooth application, it should be understood that the present invention is also useful in multiple-tooth applications, such as bridges and bars for supporting full or partial dentures. In those situations, the patient-specific abutment would not necessarily need a non-rotational feature for engaging the underlying implant(s) because the final prosthesis would also be supported by another structure in the mouth (e.g., one or more additional underlying implants), which would inherently achieve a non-rotational aspect to the design. In any event, using a scanning process to obtain the necessary information about the emergence profile shape of the gingiva and the dimensional and/or positional information for the implant(s) (via information markers in the temporary prosthetic assembly) can lead to the development of an aesthetically pleasing multiple-tooth system.

While the present invention has been described with reference to one or more particular embodiments, those skilled in the art will recognize that many changes may be made thereto without departing from the spirit and scope of the present invention. Each of these embodiments and obvious variations thereof is contemplated as falling within the spirit and scope of the present invention, which is set forth in the claims that follow.

What is claimed is:

1. A prosthesis assembly for attachment to a dental implant, comprising:

an abutment for non-rotationally mating with the dental implant, the abutment including a flange and an outer surface of the flange having a shape for shaping gingival tissue in an anatomic fashion; and

an abutment cap configured to be removably coupled to the abutment such that a bottom end of the abutment cap aligns with the flange, the abutment cap including a plurality of informational markers on a top surface of the abutment cap that provide information concerning the abutment or the dental implant to assist a user in designing a final prosthesis,

32

wherein a first informational marker of the plurality of informational markers provides one of a height or a diameter of a portion of the abutment coupled to the dental implant, and

wherein a second informational marker of the plurality of informational markers is aligned with a flat of a non-rotational feature of the abutment to indicate a location of a flat of a non-rotational feature of the dental implant when the abutment is non-rotationally coupled to the dental implant.

2. The prosthesis assembly of claim 1, further including: a temporary prosthesis removably coupled to the abutment cap.

3. The prosthesis assembly of claim 2, wherein the combination of the temporary prosthesis and the abutment cap are removably coupled to the abutment.

4. The prosthesis assembly of claim 2, wherein the temporary prosthesis has a non-round shape.

5. The prosthesis assembly of claim 1, wherein the abutment cap and the abutment are configured to have a snap fit engagement.

6. The prosthesis assembly of claim 1, wherein the abutment includes a female or male retention feature configured to mate with a corresponding female or male retention feature of the abutment cap.

7. The prosthesis assembly of claim 1, wherein the abutment includes a first anti-rotational structure configured to mate with a second anti-rotational structure of the abutment cap to non-rotationally couple the abutment with the abutment cap.

8. The prosthesis assembly of claim 1, wherein the abutment includes an anti-rotational feature for non-rotationally mating with the dental implant.

9. The prosthesis assembly of claim 1, further comprising: a fastening device configured to couple the abutment to the dental implant, the abutment including an aperture, the fastening device extending through the aperture and coupling with the dental implant.

10. The prosthesis assembly of claim 1, wherein the abutment cap has an anatomically shaped tooth structure and is a temporary prosthesis.

11. An abutment assembly for attachment to a dental implant, comprising:

an abutment having a lower region and an upper region, the lower region including an anti-rotational feature for non-rotationally mating with the dental implant;

an abutment cap configured to be coupled to the upper region of the abutment, a top surface of the abutment cap including one or more informational markers providing information concerning the abutment or the dental implant, wherein the one or more informational markers include at least one of a groove and projection on the top surface; and

a temporary prosthesis removably coupled to the abutment cap, wherein the temporary prosthesis has an internal surface that has a shape that mates with the one or more informational markers for non-rotationally mating with the abutment cap.

12. The abutment assembly of claim 11, the abutment cap and the abutment are configured to have a snap fit engagement.

13. The abutment assembly of claim 11, wherein the abutment includes a female or male retention feature configured to mate with a corresponding female or male retention feature of the abutment cap.

14. The abutment assembly of claim 11, wherein the abutment includes a first anti-rotational structure configured



to mate with a second anti-rotational structure of the abutment cap to non-rotationally couple the abutment with the abutment cap.

**15.** The abutment assembly of claim **11**, wherein the abutment includes an anti-rotational feature for non-rotationally mating with the dental implant. 5

**16.** The abutment assembly of claim **11**, further comprising:

a fastening device configured to couple the abutment to the dental implant, the abutment including an aperture, 10  
the fastening device extending through the aperture and coupling with the dental implant.

\* \* \* \* \*



UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : 11,389,275 B2  
APPLICATION NO. : 16/445978  
DATED : July 19, 2022  
INVENTOR(S) : T. Tait Robb et al.


Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Claims

Column 32, Line 59, Claim 12 after “The abutment assembly of claim 11,” insert --wherein-- therein.

Signed and Sealed this  
Twenty-seventh Day of September, 2022

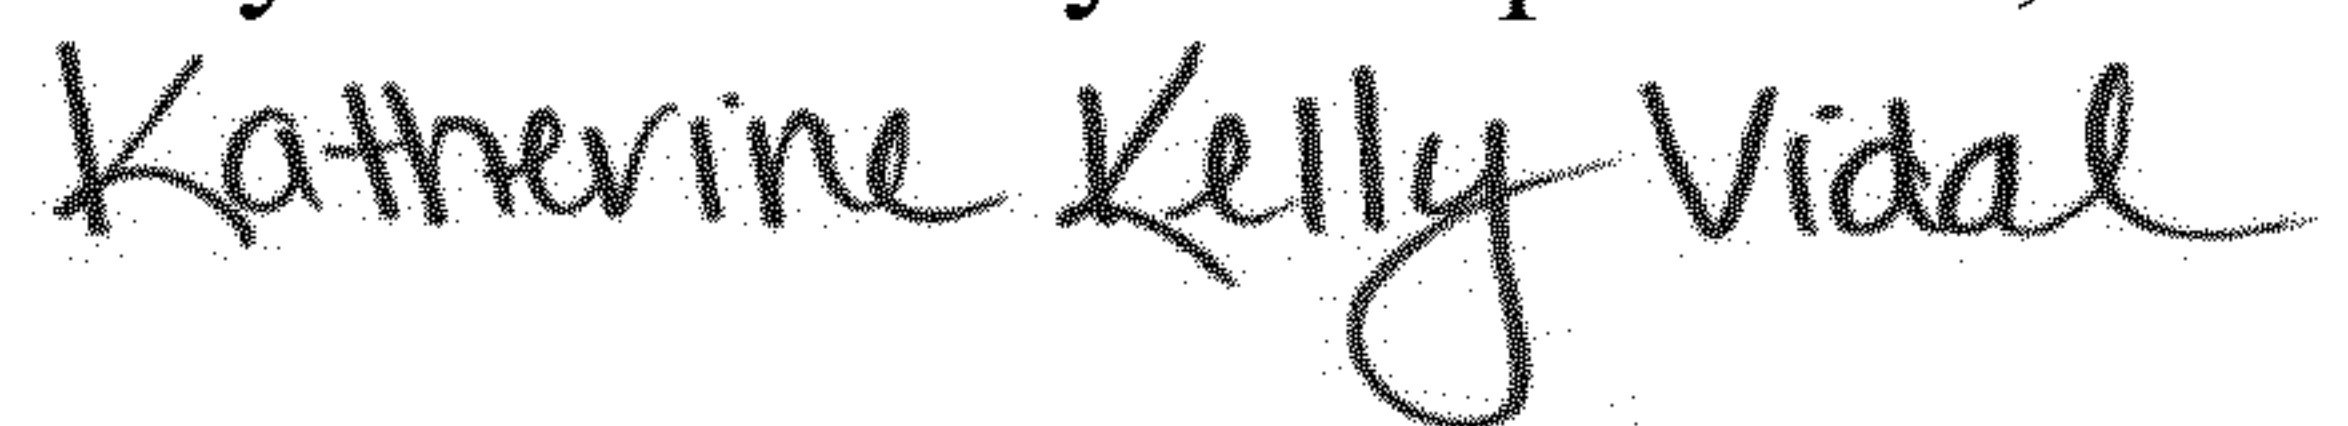

Katherine Kelly Vidal  
*Director of the United States Patent and Trademark Office*