

US011607185B2

(12) **United States Patent**
Gregerson et al.

(10) **Patent No.:** **US 11,607,185 B2**
(45) **Date of Patent:** **Mar. 21, 2023**

(54) **CANTILEVERED X-RAY CT SYSTEM FOR MULTI-AXIS IMAGING**

(71) Applicant: **Mobius Imaging, LLC**, Shirley, MA (US)

(72) Inventors: **Eugene A. Gregerson**, Bolton, MA (US); **Russell Stanton**, Lunenburg, MA (US); **Michael Connor**, Dunstable, MA (US); **Paul Sebring**, Townsend, MA (US)

(73) Assignee: **Mobius Imaging, LLC**, Shirley, MA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 65 days.

(21) Appl. No.: **17/201,440**

(22) Filed: **Mar. 15, 2021**

(65) **Prior Publication Data**

US 2021/0196216 A1 Jul. 1, 2021

Related U.S. Application Data

(63) Continuation of application No. 16/818,060, filed on Mar. 13, 2020, now Pat. No. 10,973,478, which is a (Continued)

(51) **Int. Cl.**
A61B 6/02 (2006.01)
A61B 6/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 6/4476** (2013.01); **A61B 6/00** (2013.01); **A61B 6/03** (2013.01); **A61B 6/035** (2013.01);
(Continued)

(58) **Field of Classification Search**
None
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,961,208 A 10/1990 Okada
5,448,607 A 9/1995 McKenna
(Continued)

FOREIGN PATENT DOCUMENTS

CN 104169507 A 11/2014
DE 19846980 A1 10/1999
(Continued)

OTHER PUBLICATIONS


Ergun, "Equina.TM.: A CT Scanner Designed by and for Veterinarians", Asto CT, 12 pages, (Nov. 24, 2016).
(Continued)

Primary Examiner — Hoon K Song
(74) *Attorney, Agent, or Firm* — Howard & Howard Attorneys PLLC

(57) **ABSTRACT**

A multi-axis imaging system comprising an imaging gantry with an imaging axis extending through a bore of the imaging gantry, a support column that supports the imaging gantry on one side of the gantry in a cantilevered manner, and a base that supports the imaging gantry and the support column. The imaging system including a first drive mechanism that translates the gantry in a vertical direction relative to the support column and the base, a second drive mechanism that rotates the gantry with respect to the support column between a first orientation where the imaging axis of the imaging gantry extends in a vertical direction parallel to the support column and a second orientation where the imaging axis of the gantry extends in a horizontal direction parallel with the base, and a third drive mechanism that translates the support column and the gantry in a horizontal direction along the base.

18 Claims, 29 Drawing Sheets

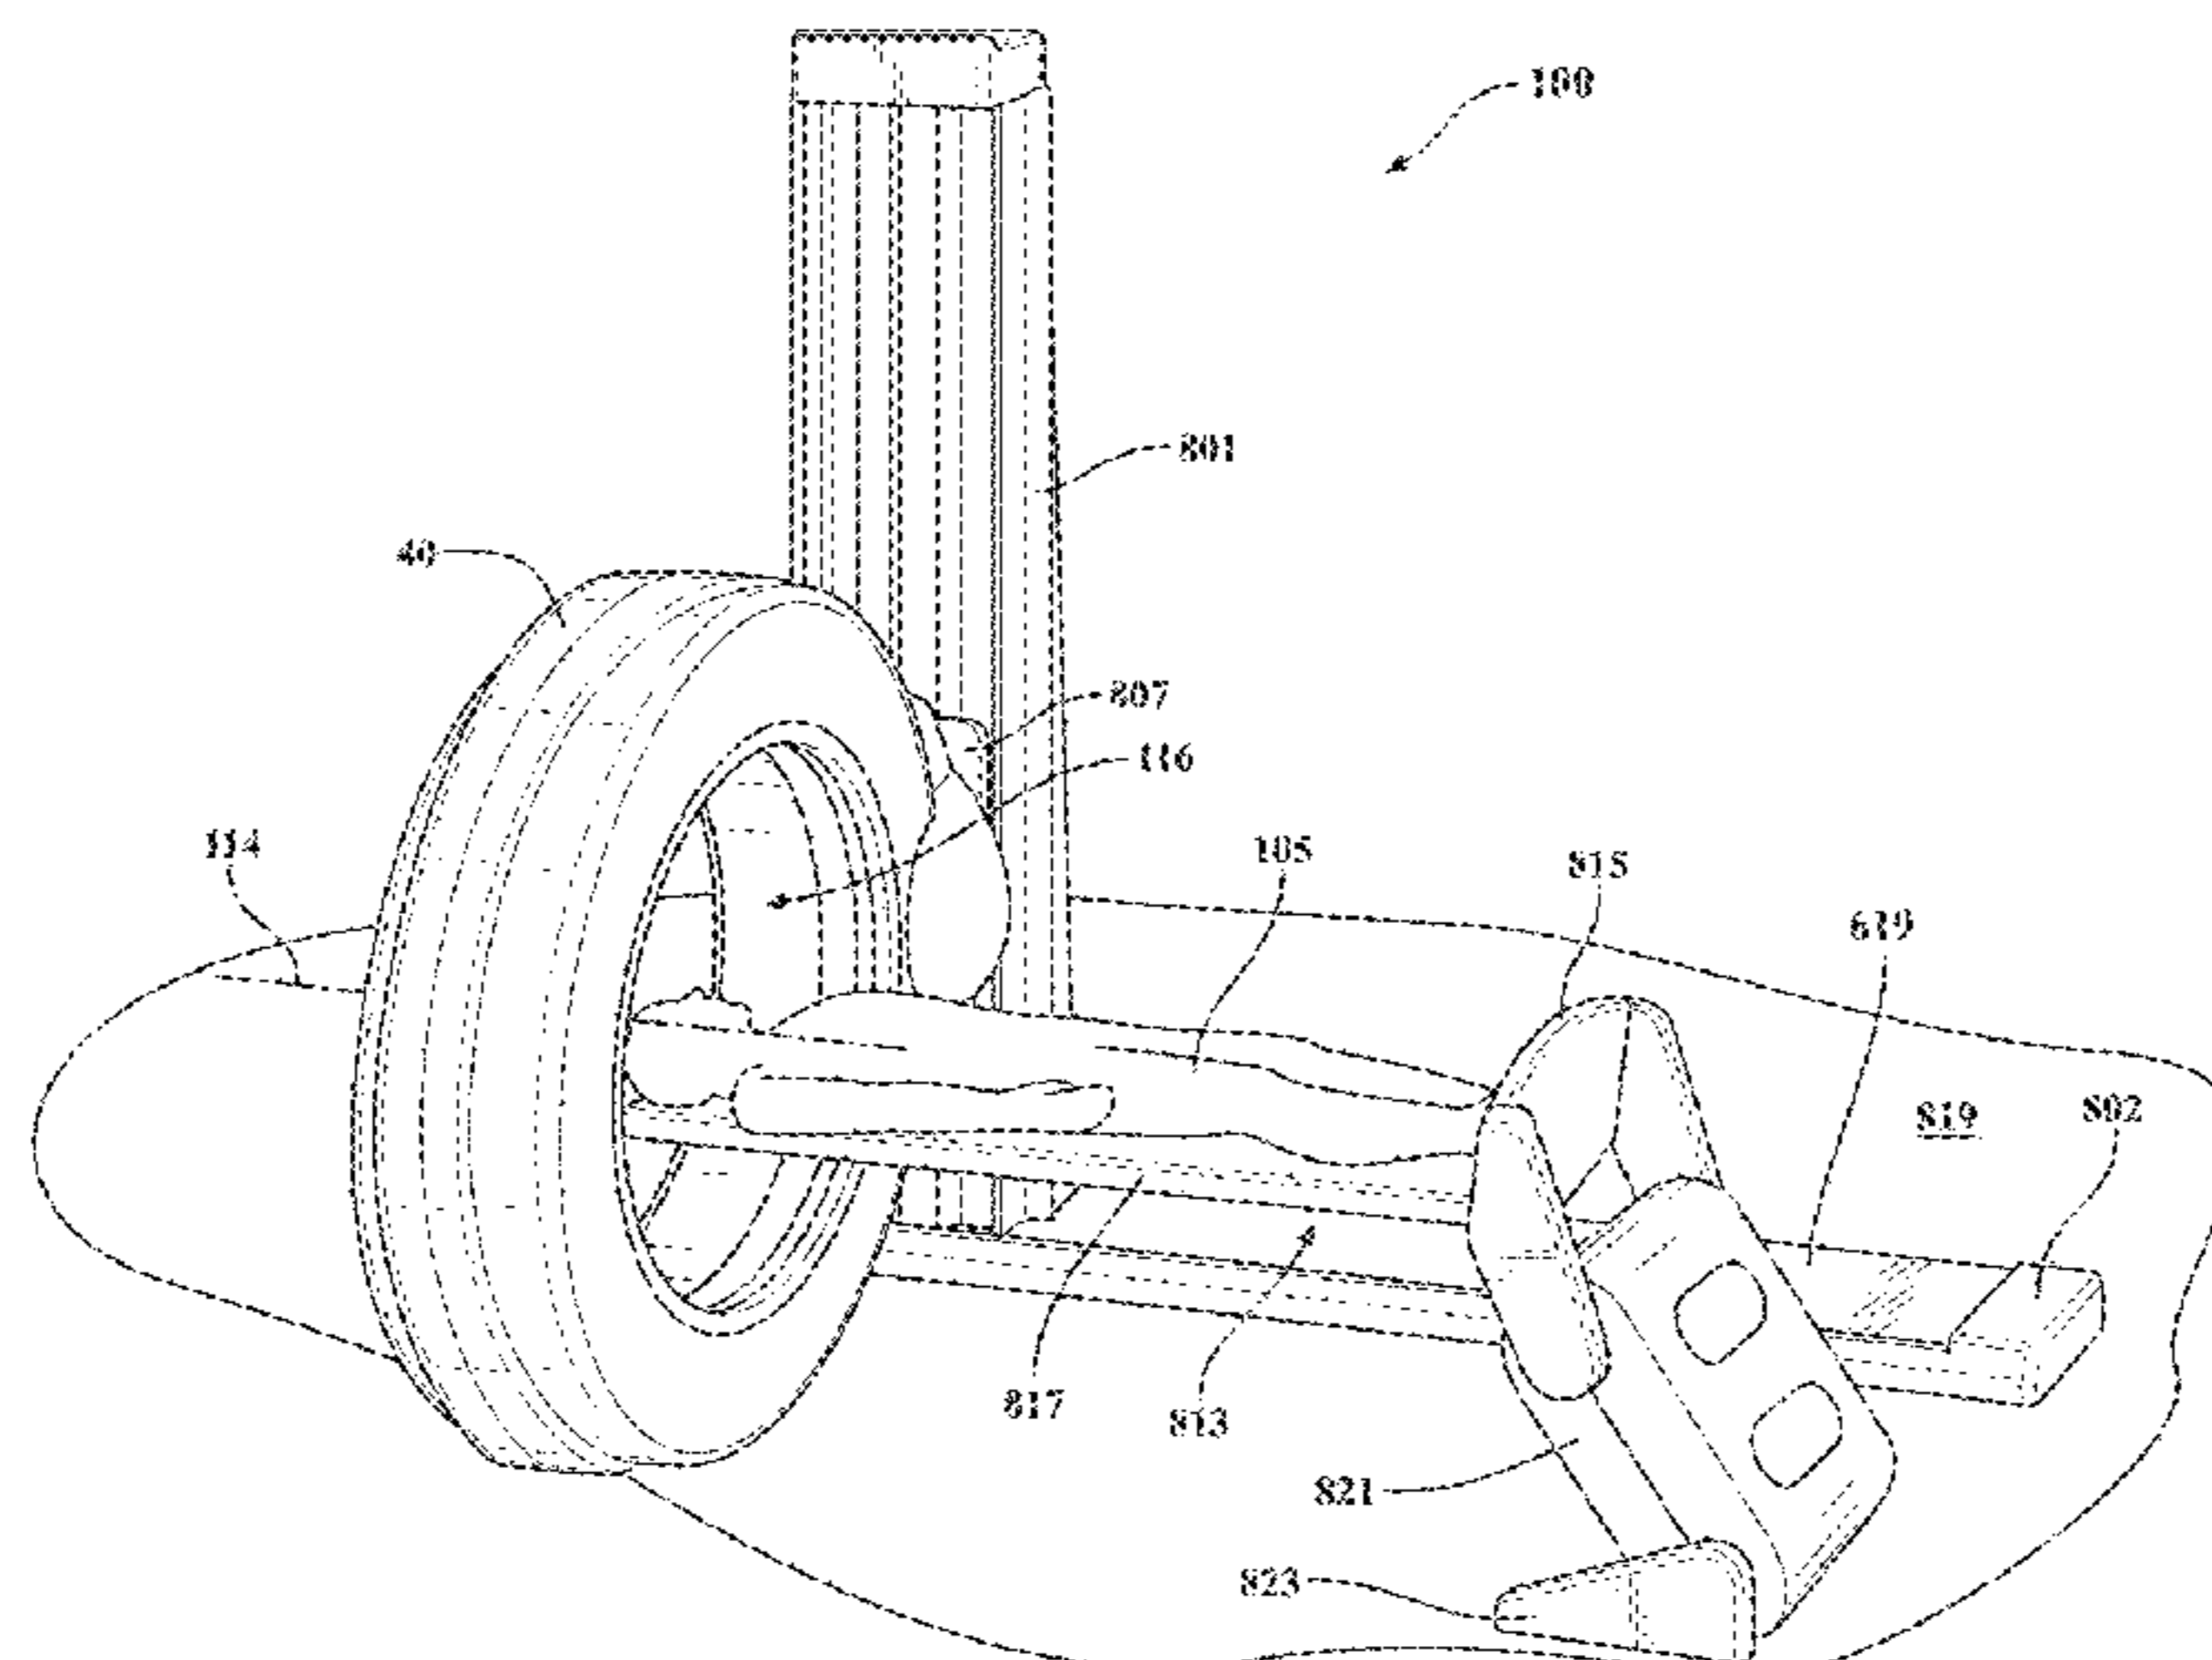

Related U.S. Application Data

continuation of application No. 15/817,672, filed on Nov. 20, 2017, now Pat. No. 10,624,596.

(60) Provisional application No. 62/425,746, filed on Nov. 23, 2016.

(51) **Int. Cl.**

A61B 6/04 (2006.01)
A61B 6/03 (2006.01)
B25J 19/00 (2006.01)
B25J 15/00 (2006.01)
B25J 5/02 (2006.01)
B25J 9/10 (2006.01)
B25J 9/16 (2006.01)
B25J 9/00 (2006.01)
A61B 5/055 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 6/0407* (2013.01); *A61B 6/4447* (2013.01); *A61B 6/4458* (2013.01); *A61B 6/504* (2013.01); *A61B 6/505* (2013.01); *A61B 6/508* (2013.01); *A61B 5/055* (2013.01); *A61B 6/037* (2013.01); *B25J 5/02* (2013.01); *B25J 9/0096* (2013.01); *B25J 9/104* (2013.01); *B25J 9/1676* (2013.01); *B25J 15/0019* (2013.01); *B25J 19/0075* (2013.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,574,763 A 11/1996 Dehner
 5,574,769 A 11/1996 Dehner
 6,102,567 A 8/2000 Cabral et al.
 6,246,239 B1 6/2001 Krogmann et al.
 6,735,274 B1 5/2004 Zahavi et al.
 6,794,871 B2 9/2004 Imai et al.
 7,224,764 B2 5/2007 Sukovic et al.
 7,456,407 B2 11/2008 Stark
 7,607,832 B2 10/2009 Jensen et al.
 7,796,730 B2 9/2010 Marash et al.
 7,806,589 B2 10/2010 Tashman et al.
 7,944,208 B2 5/2011 Dutto et al.
 8,118,488 B2 2/2012 Gregerson
 9,301,726 B2 4/2016 Mackie et al.
 9,320,941 B2 4/2016 Garside
 10,624,596 B2 4/2020 Gregerson et al.
 2004/0170254 A1 9/2004 Gregerson et al.
 2005/0053186 A1 3/2005 Sukovic et al.
 2008/0123819 A1 5/2008 Jensen et al.
 2008/0224051 A1 9/2008 Conwell
 2009/0289663 A1 11/2009 Sogomonyan et al.
 2010/0172468 A1 7/2010 Gregerson
 2011/0200175 A1 8/2011 Gregerson et al.
 2011/0222667 A1 9/2011 Gregerson et al.
 2011/0228901 A1 9/2011 Yorkston et al.

2011/0228910 A1 9/2011 Gregerson et al.
 2012/0099697 A1* 4/2012 Helm A61B 6/50
 378/4
 2012/0256099 A1 10/2012 Gregerson et al.
 2012/0324648 A1 12/2012 Amano
 2013/0343509 A1 12/2013 Gregerson et al.
 2014/0139215 A1 5/2014 Gregerson et al.
 2015/0313557 A1* 11/2015 Mackie A61B 6/032
 378/14
 2016/0128653 A1 5/2016 Fortuna et al.
 2018/0028127 A1 2/2018 Litzenberger et al.
 2018/0055707 A1 3/2018 Stanton
 2018/0177473 A1 6/2018 Gregerson et al.
 2020/0268332 A1 8/2020 Gregerson et al.

FOREIGN PATENT DOCUMENTS

EP 0067933 A1 12/1982
 EP 0495137 A1 7/1992
 JP H02123211 U 10/1990
 JP H04352948 A 12/1992
 JP 2000214263 A 8/2000
 JP 2000312674 A 11/2000
 JP 200137747 A 2/2001
 JP 2008278902 A 11/2008
 TW 532308 U 5/2003
 WO 2007141221 A1 12/2007
 WO 2011111119 A1 9/2011
 WO 2011135191 A1 11/2011

OTHER PUBLICATIONS

Ergun, et al., Preventing equine fractures with safe, high-quality CT imaging: The Asto CT Equina.TM., White Paper, www.astoct.com, 2 pages.
 First Office Action from the European Patent Office in Application No. 13 804 681.8-1124 based on related Application No. PCT/US2013/045563, dated Jan. 9, 2018.
 International Preliminary Report on Patentability (Chapter 1 of the Patent Cooperation Treaty) and Written Opinion of the International Search Authority in related International Application No. PCT/US2017/062776 dated Jun. 6, 2019.
 International Preliminary Report on Patentability (Chapter 1 of the Patent Cooperation Treaty) in International Application No. PCT/US2013/045563 dated Dec. 24, 2014.
 International Search Report and Written Opinion issued in PCT Application No. PCT/US2013/045563 dated Sep. 16, 2013.
 Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority in related application No. PCT/US2017/062776 dated Feb. 13, 2018.
 Supplementary European Search Report from the Munich Patent Office for Application No. 13804681.8-1660/2861148 in International Application No. PCT/US2013/045563 dated Dec. 17, 2015.
 English language abstract for CN 104169507 A extracted from espacenet.com database on Nov. 21, 2022, 2 pages.
 Machine-assisted English language abstract and machine-assisted English translation for TW 532308 U extracted from Google Translate on Nov. 21, 2022, 13 pages.

* cited by examiner

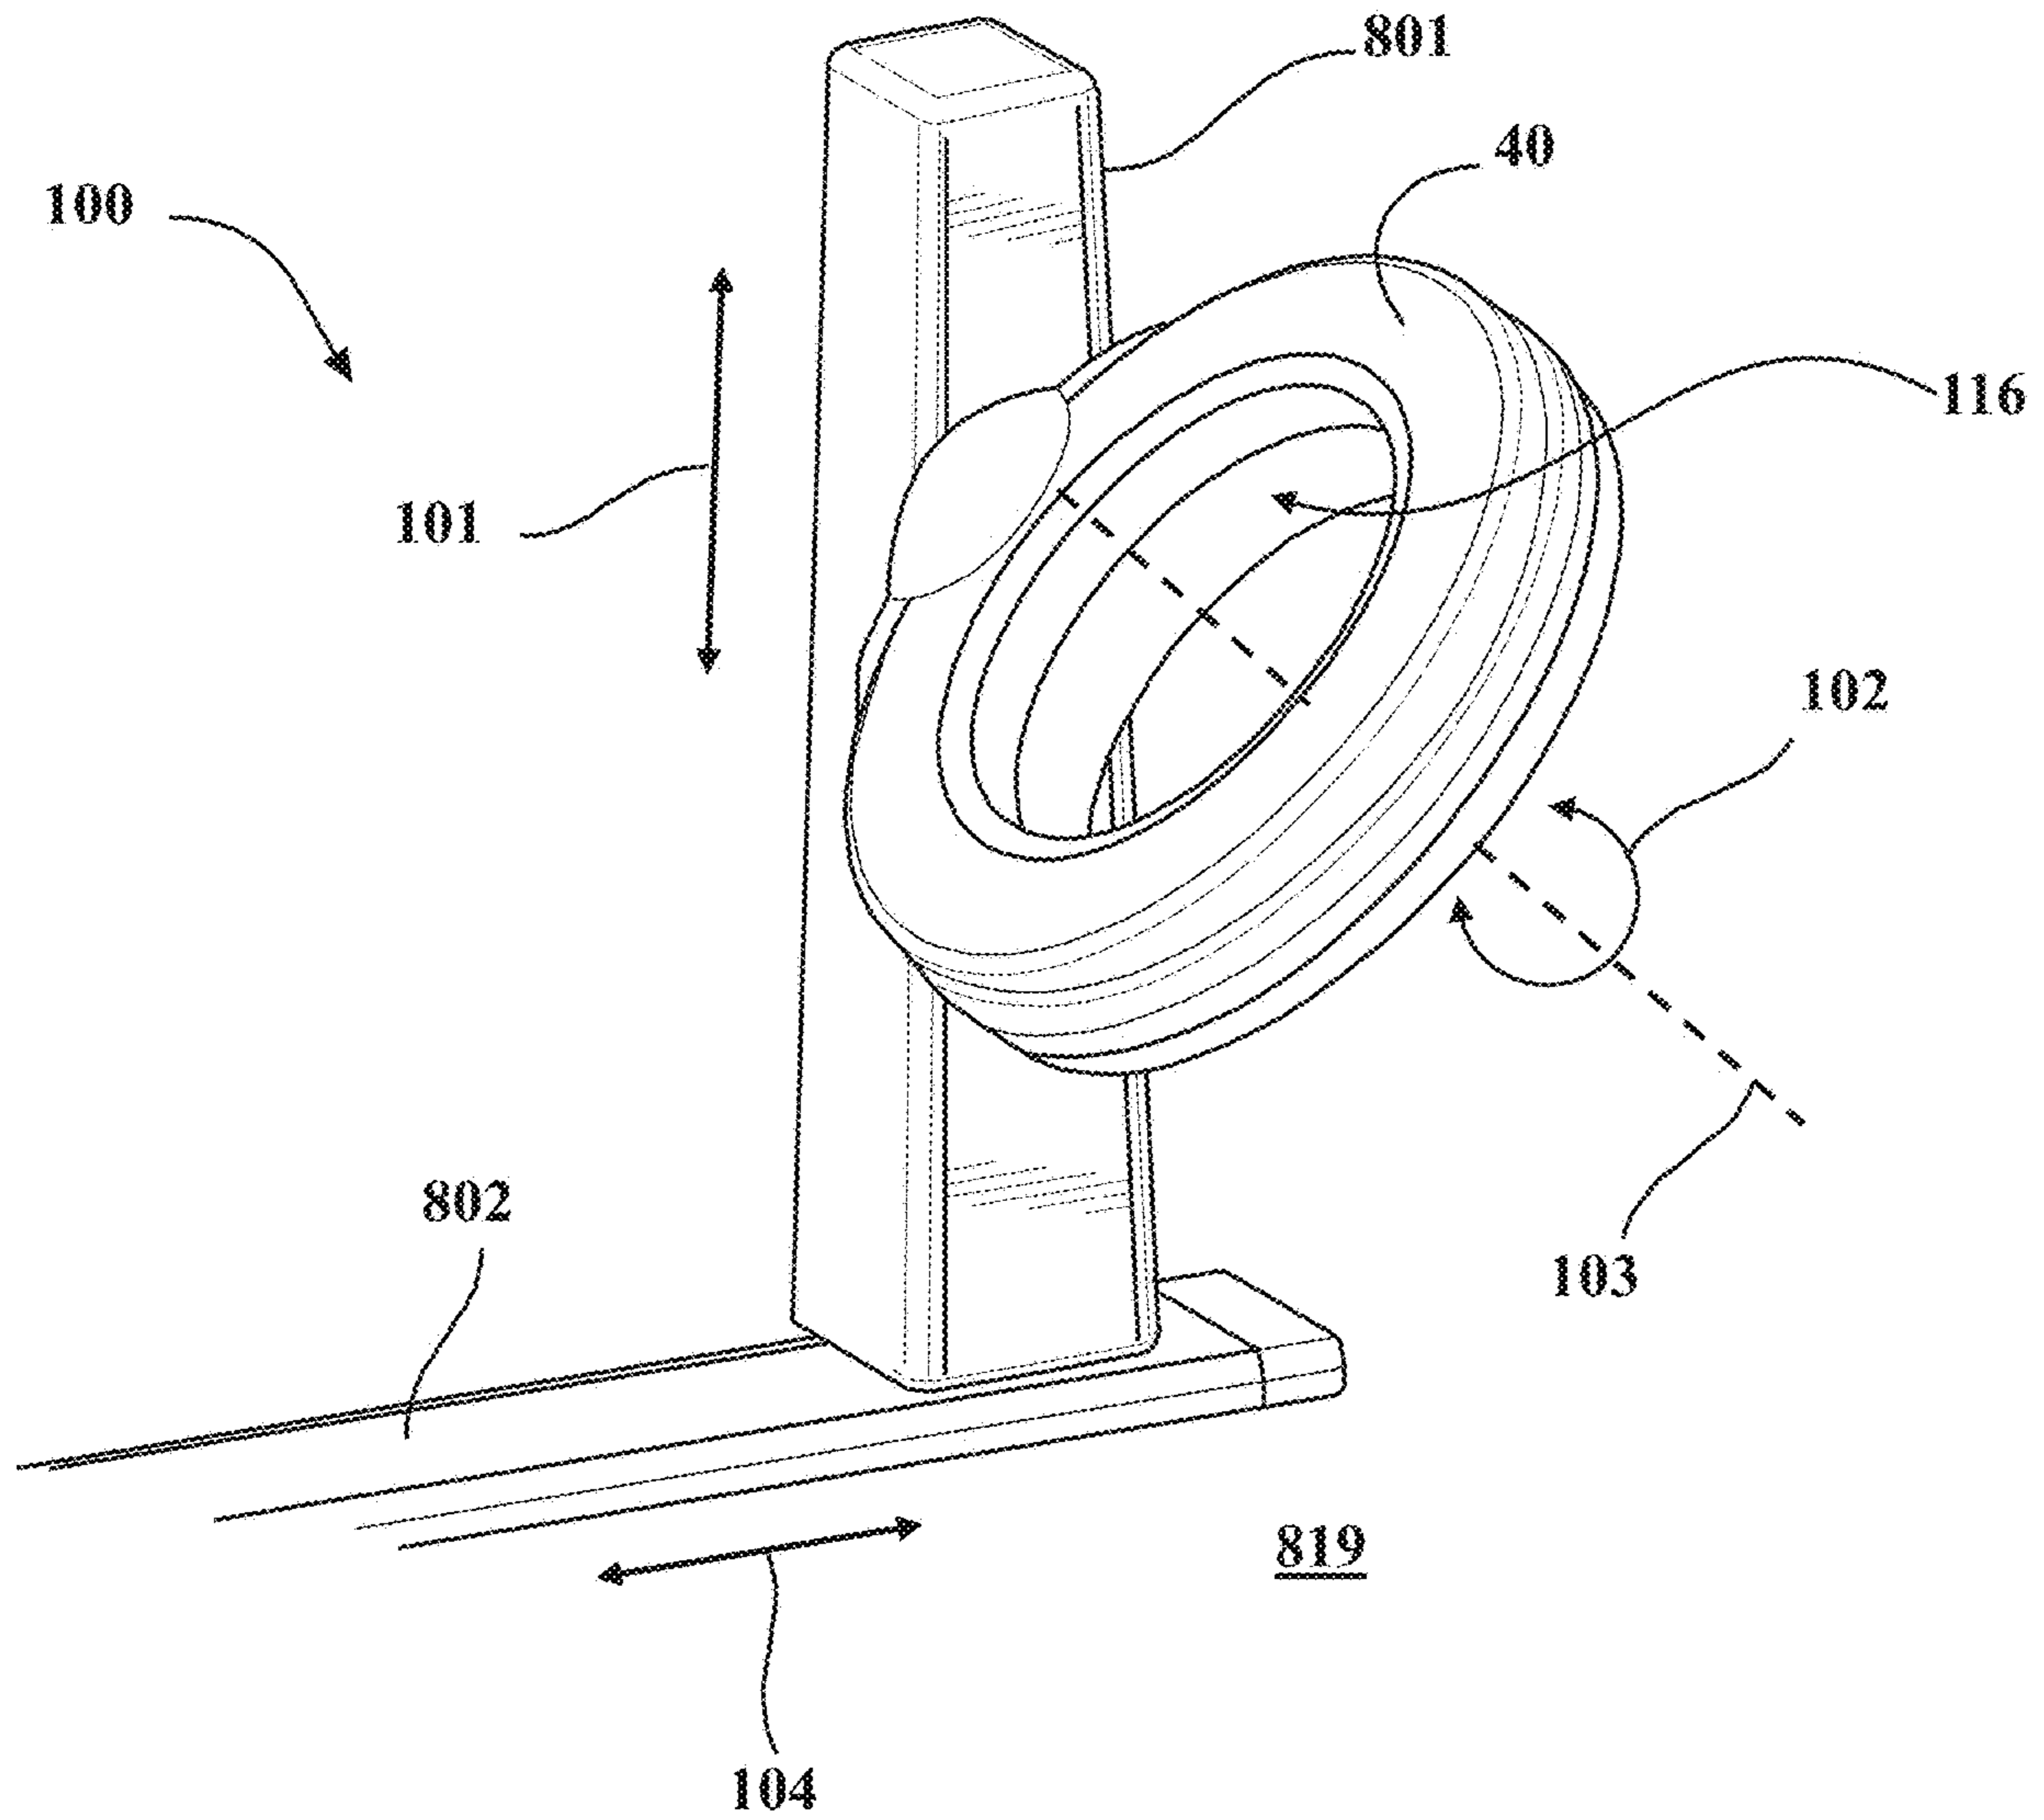


FIG. 1

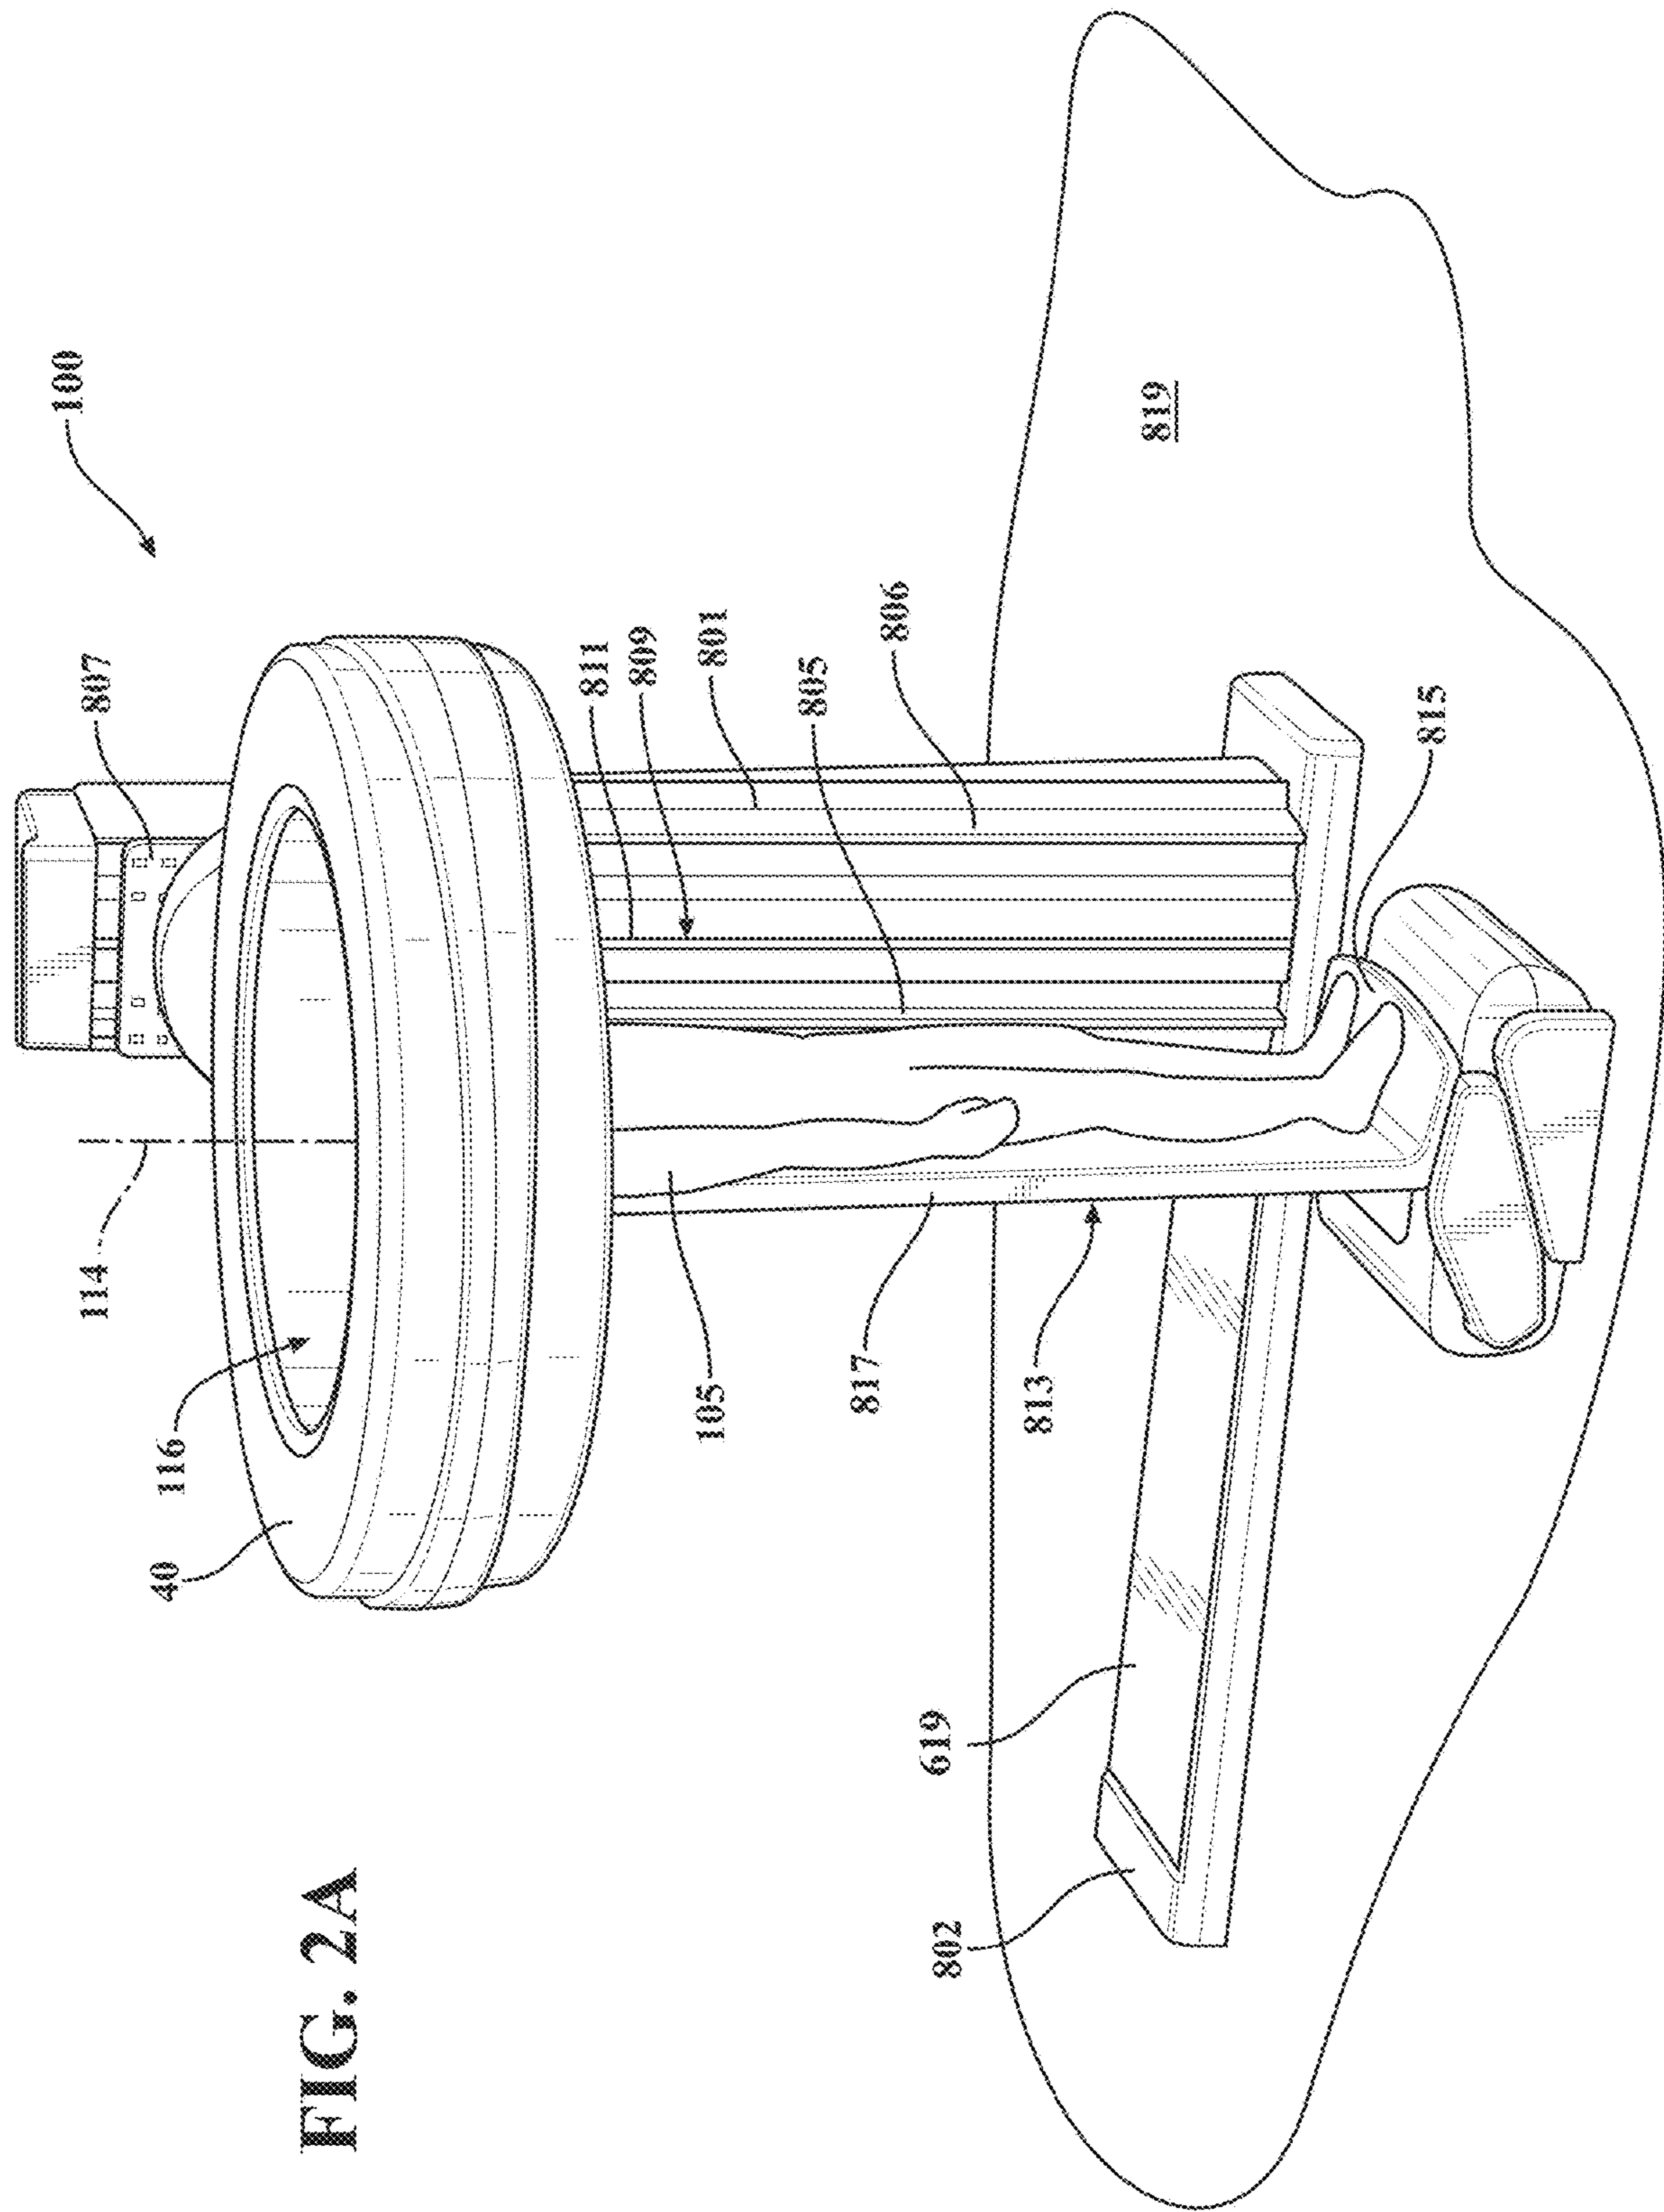


FIG. 2A

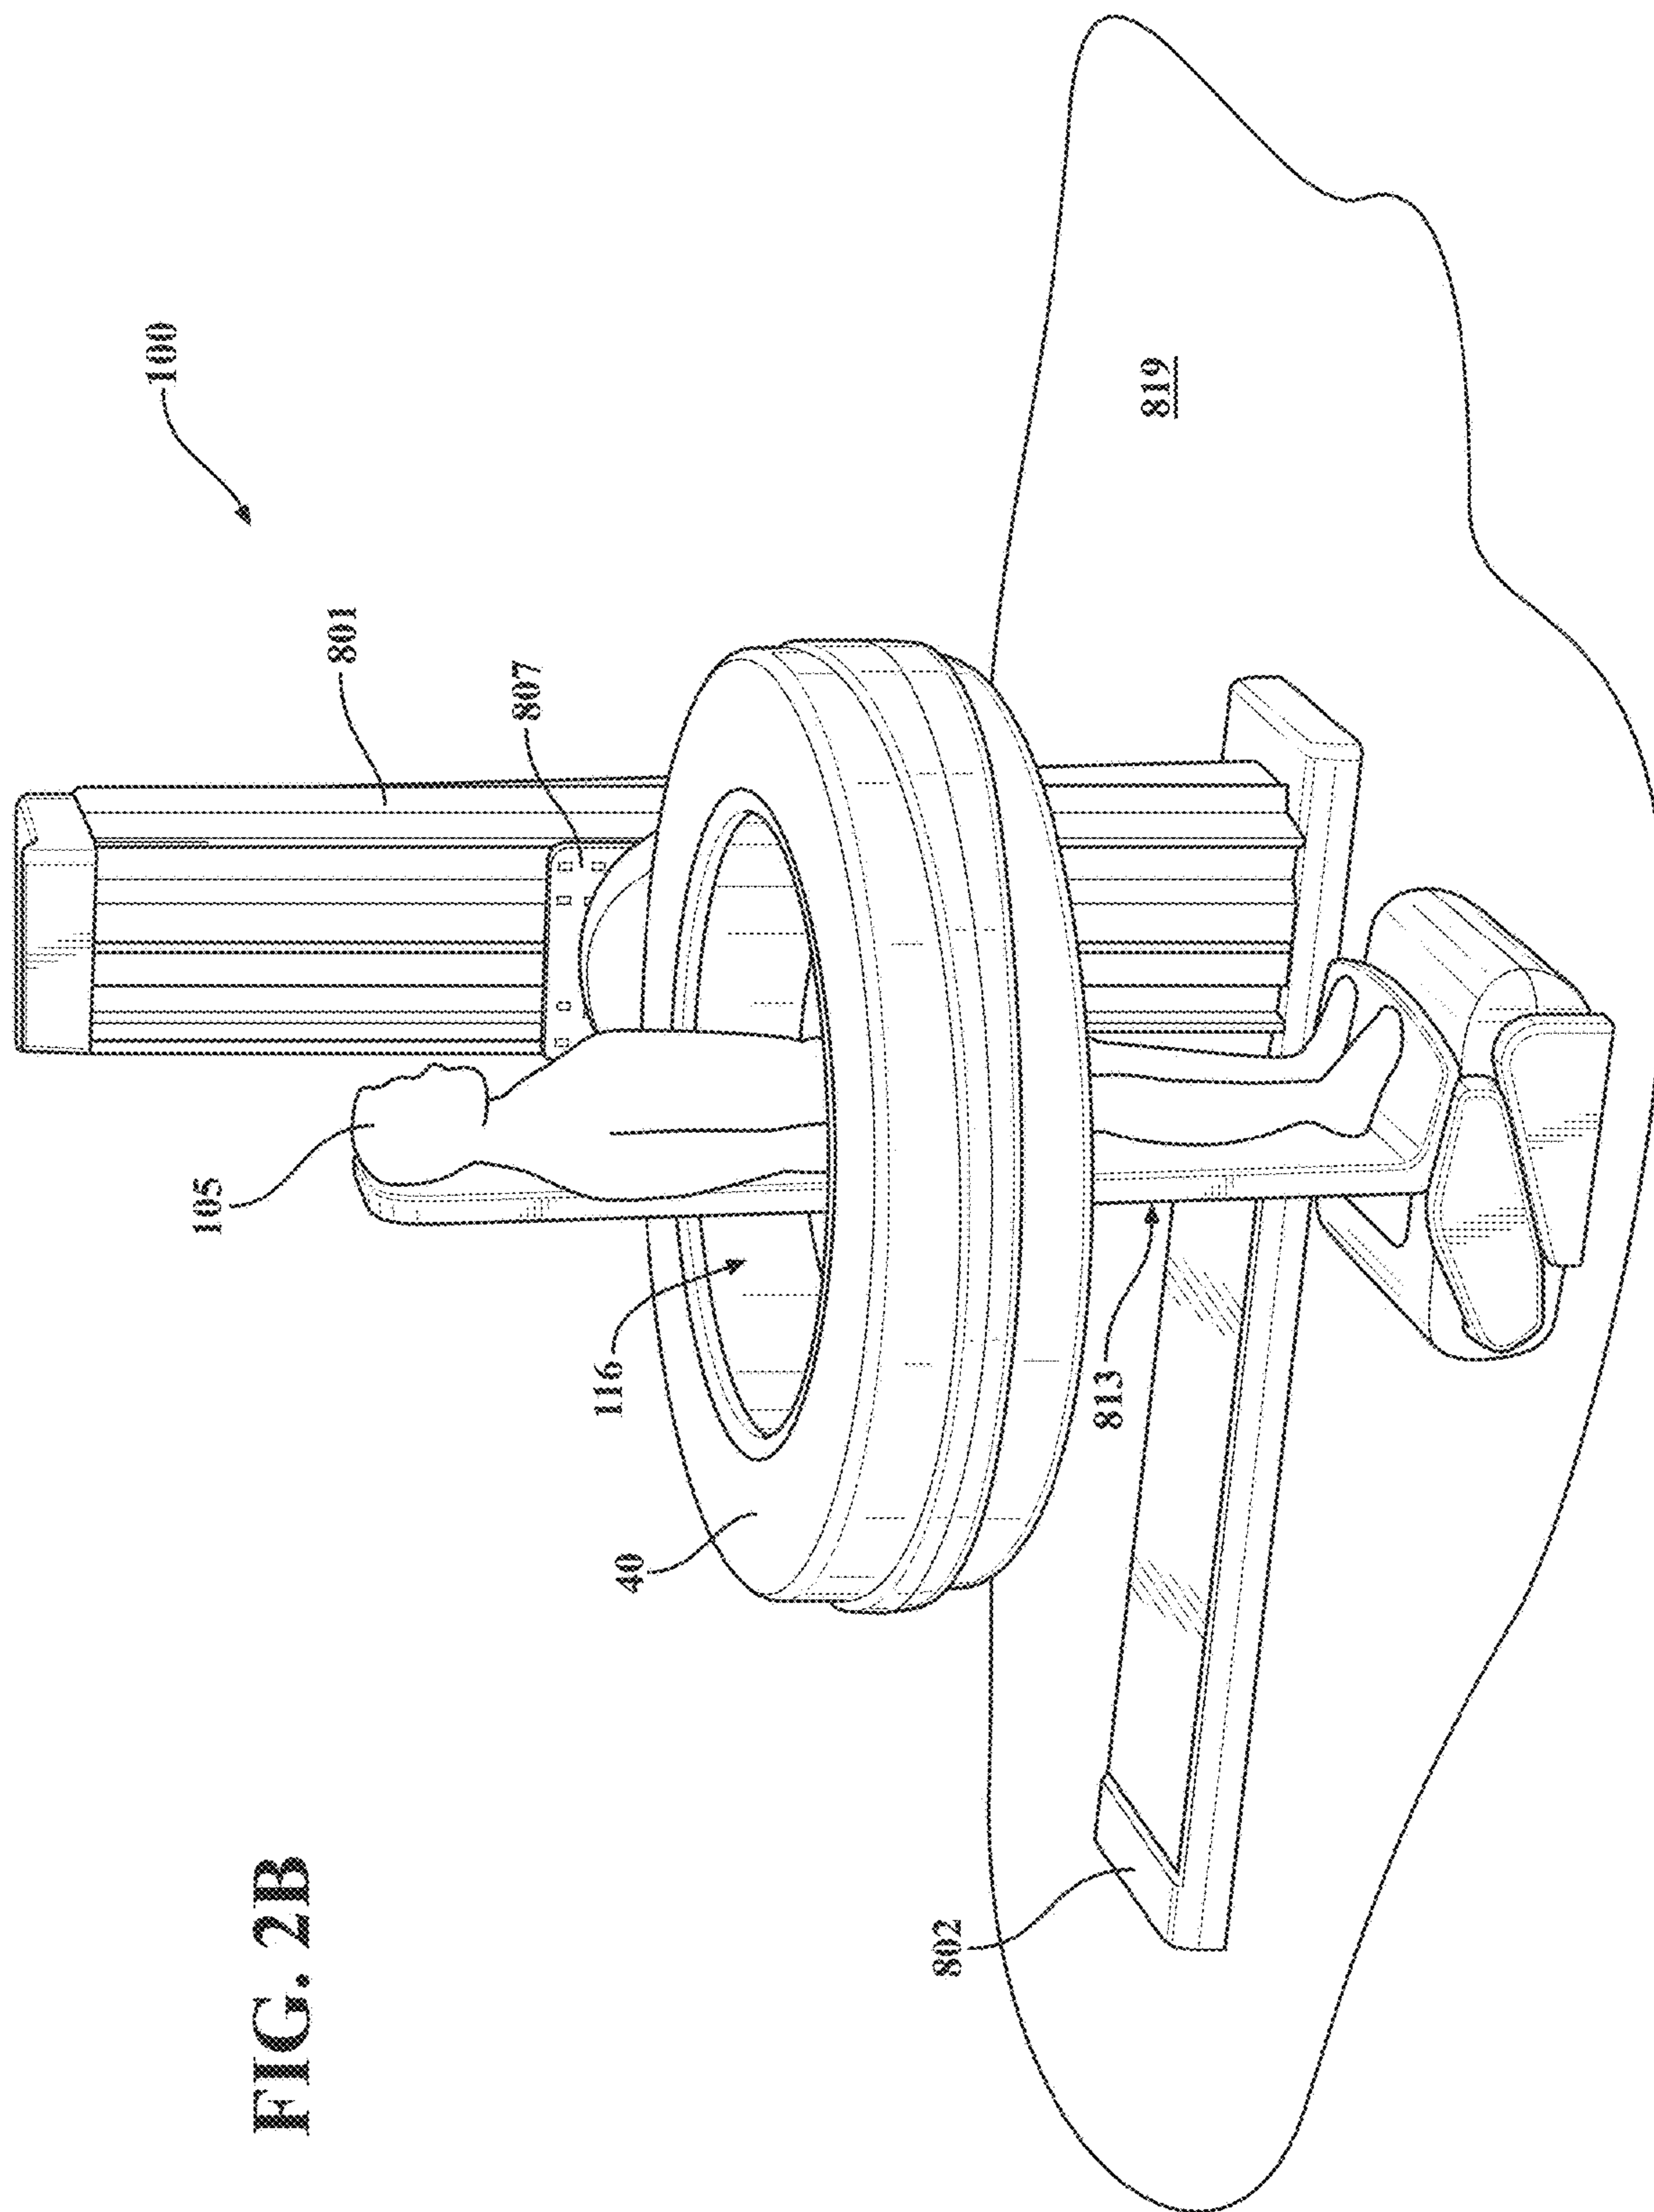


FIG. 2B

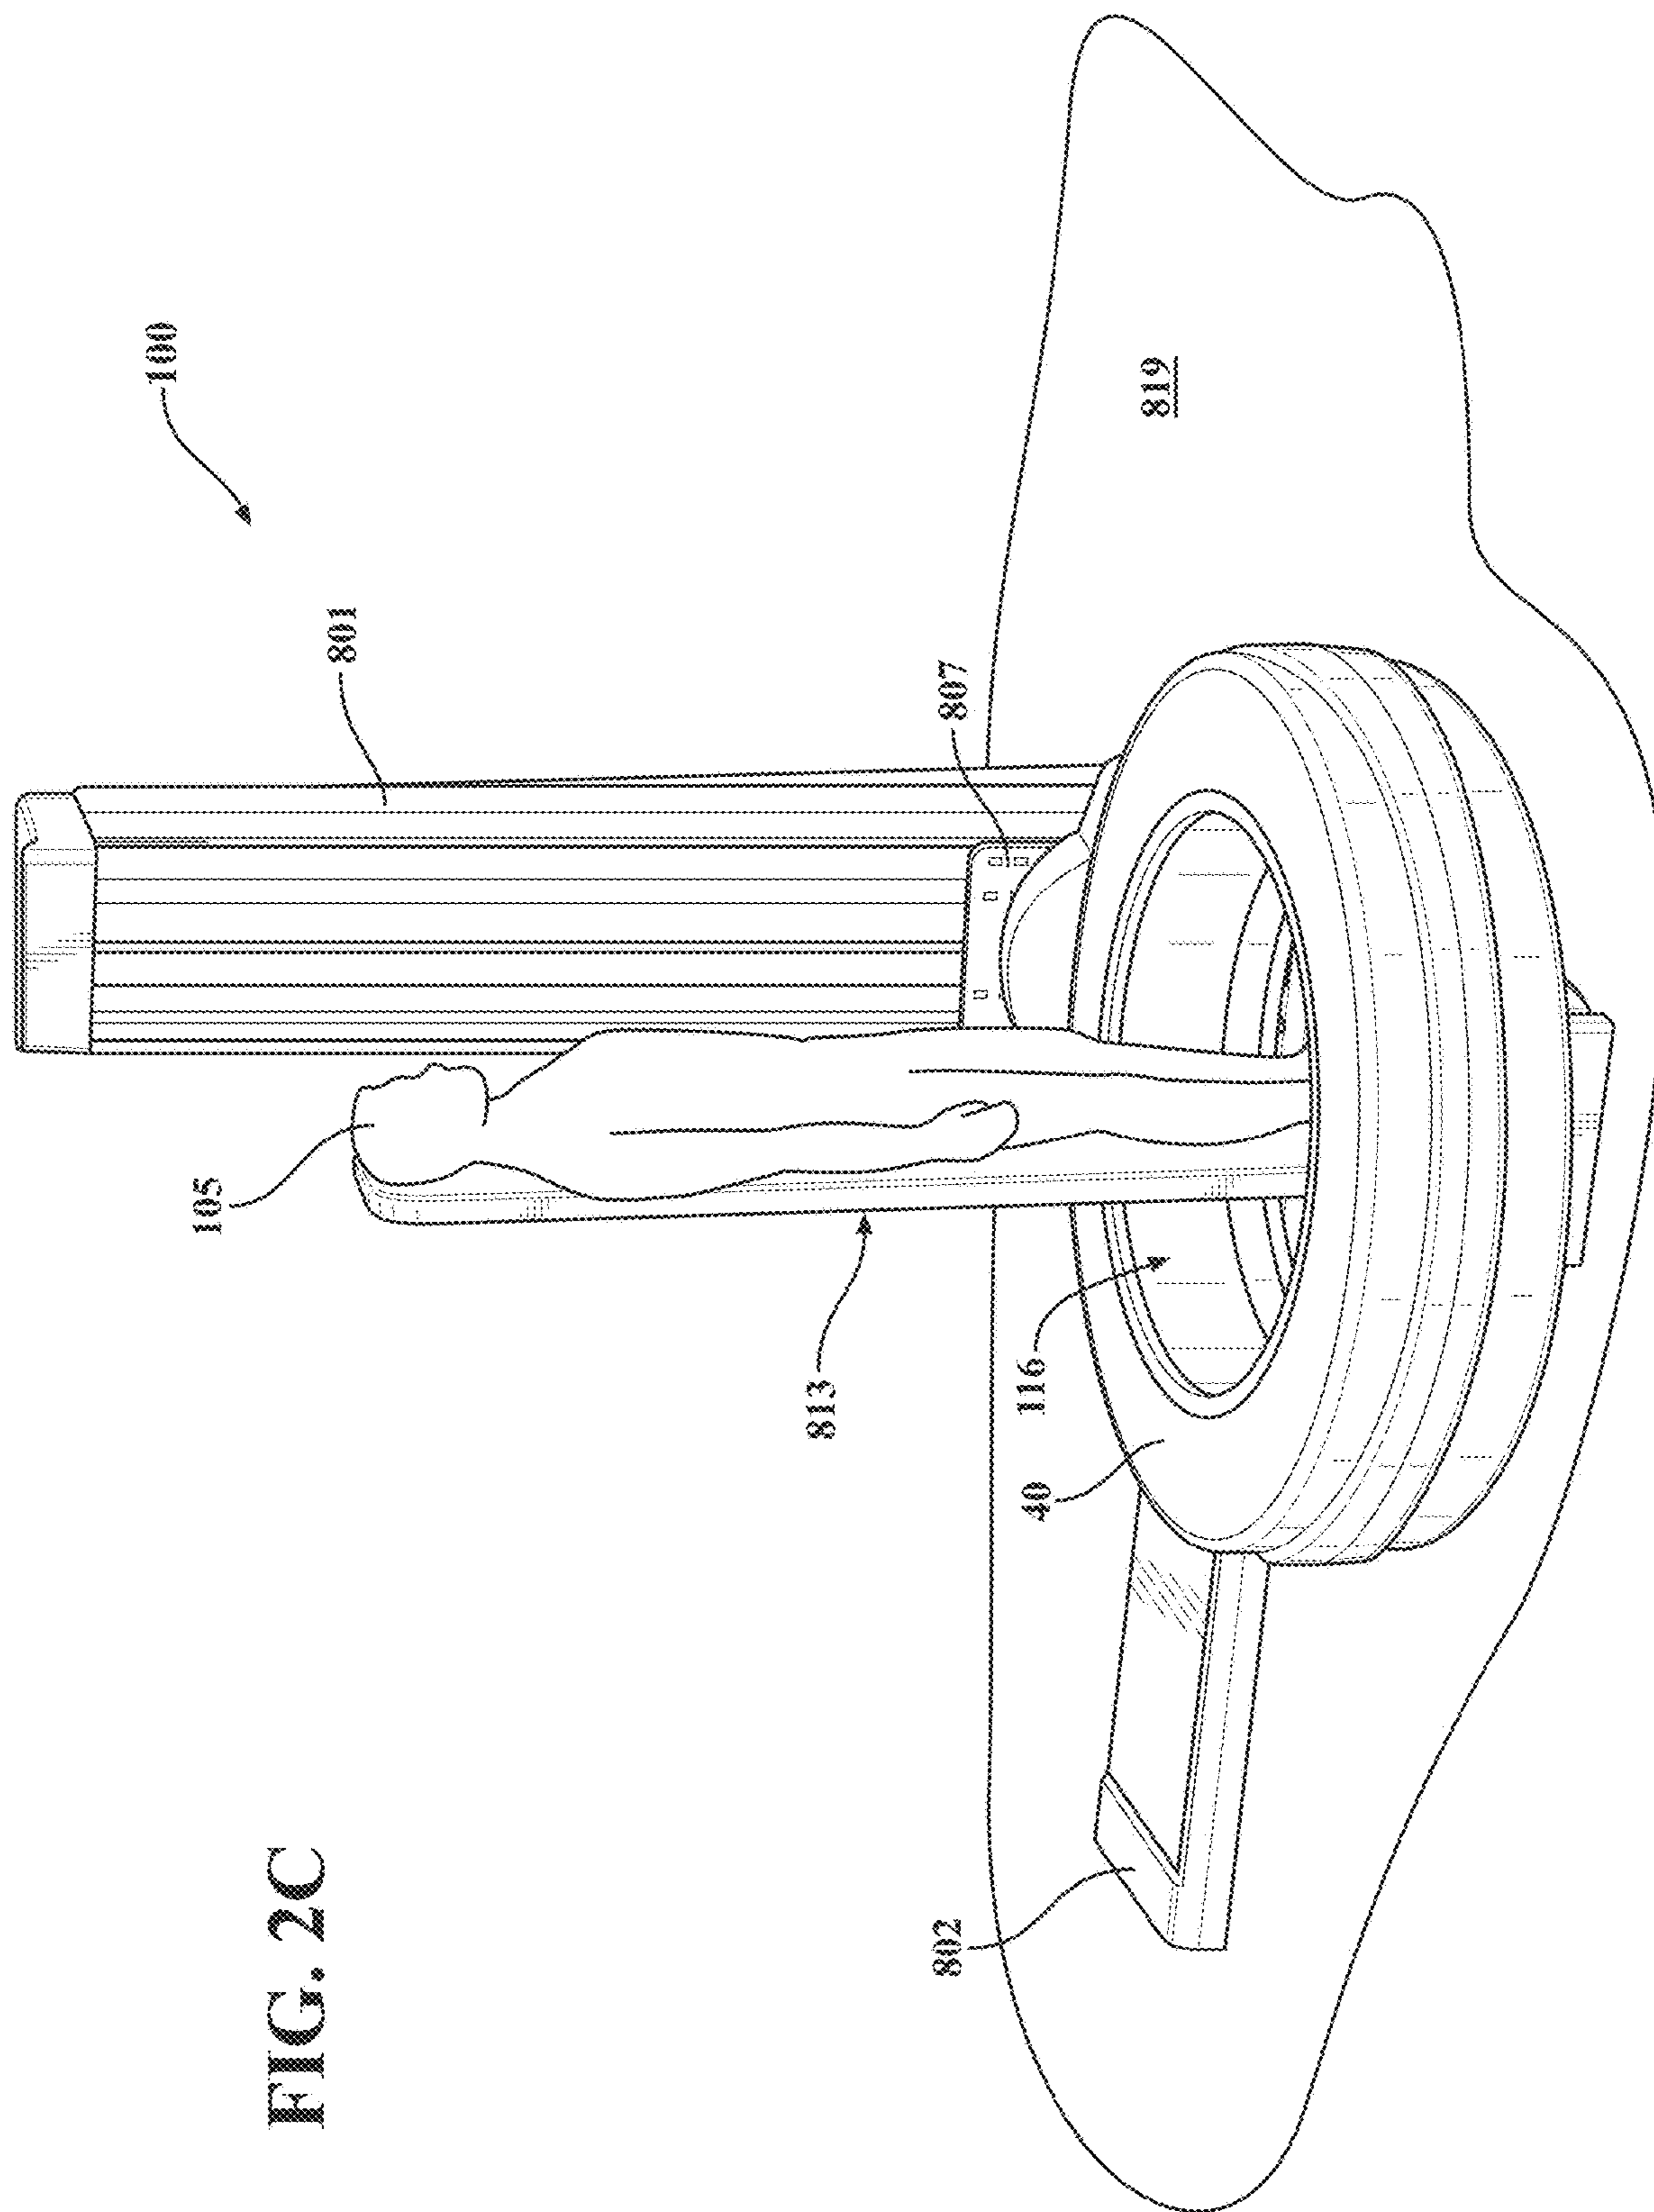


FIG. 2C

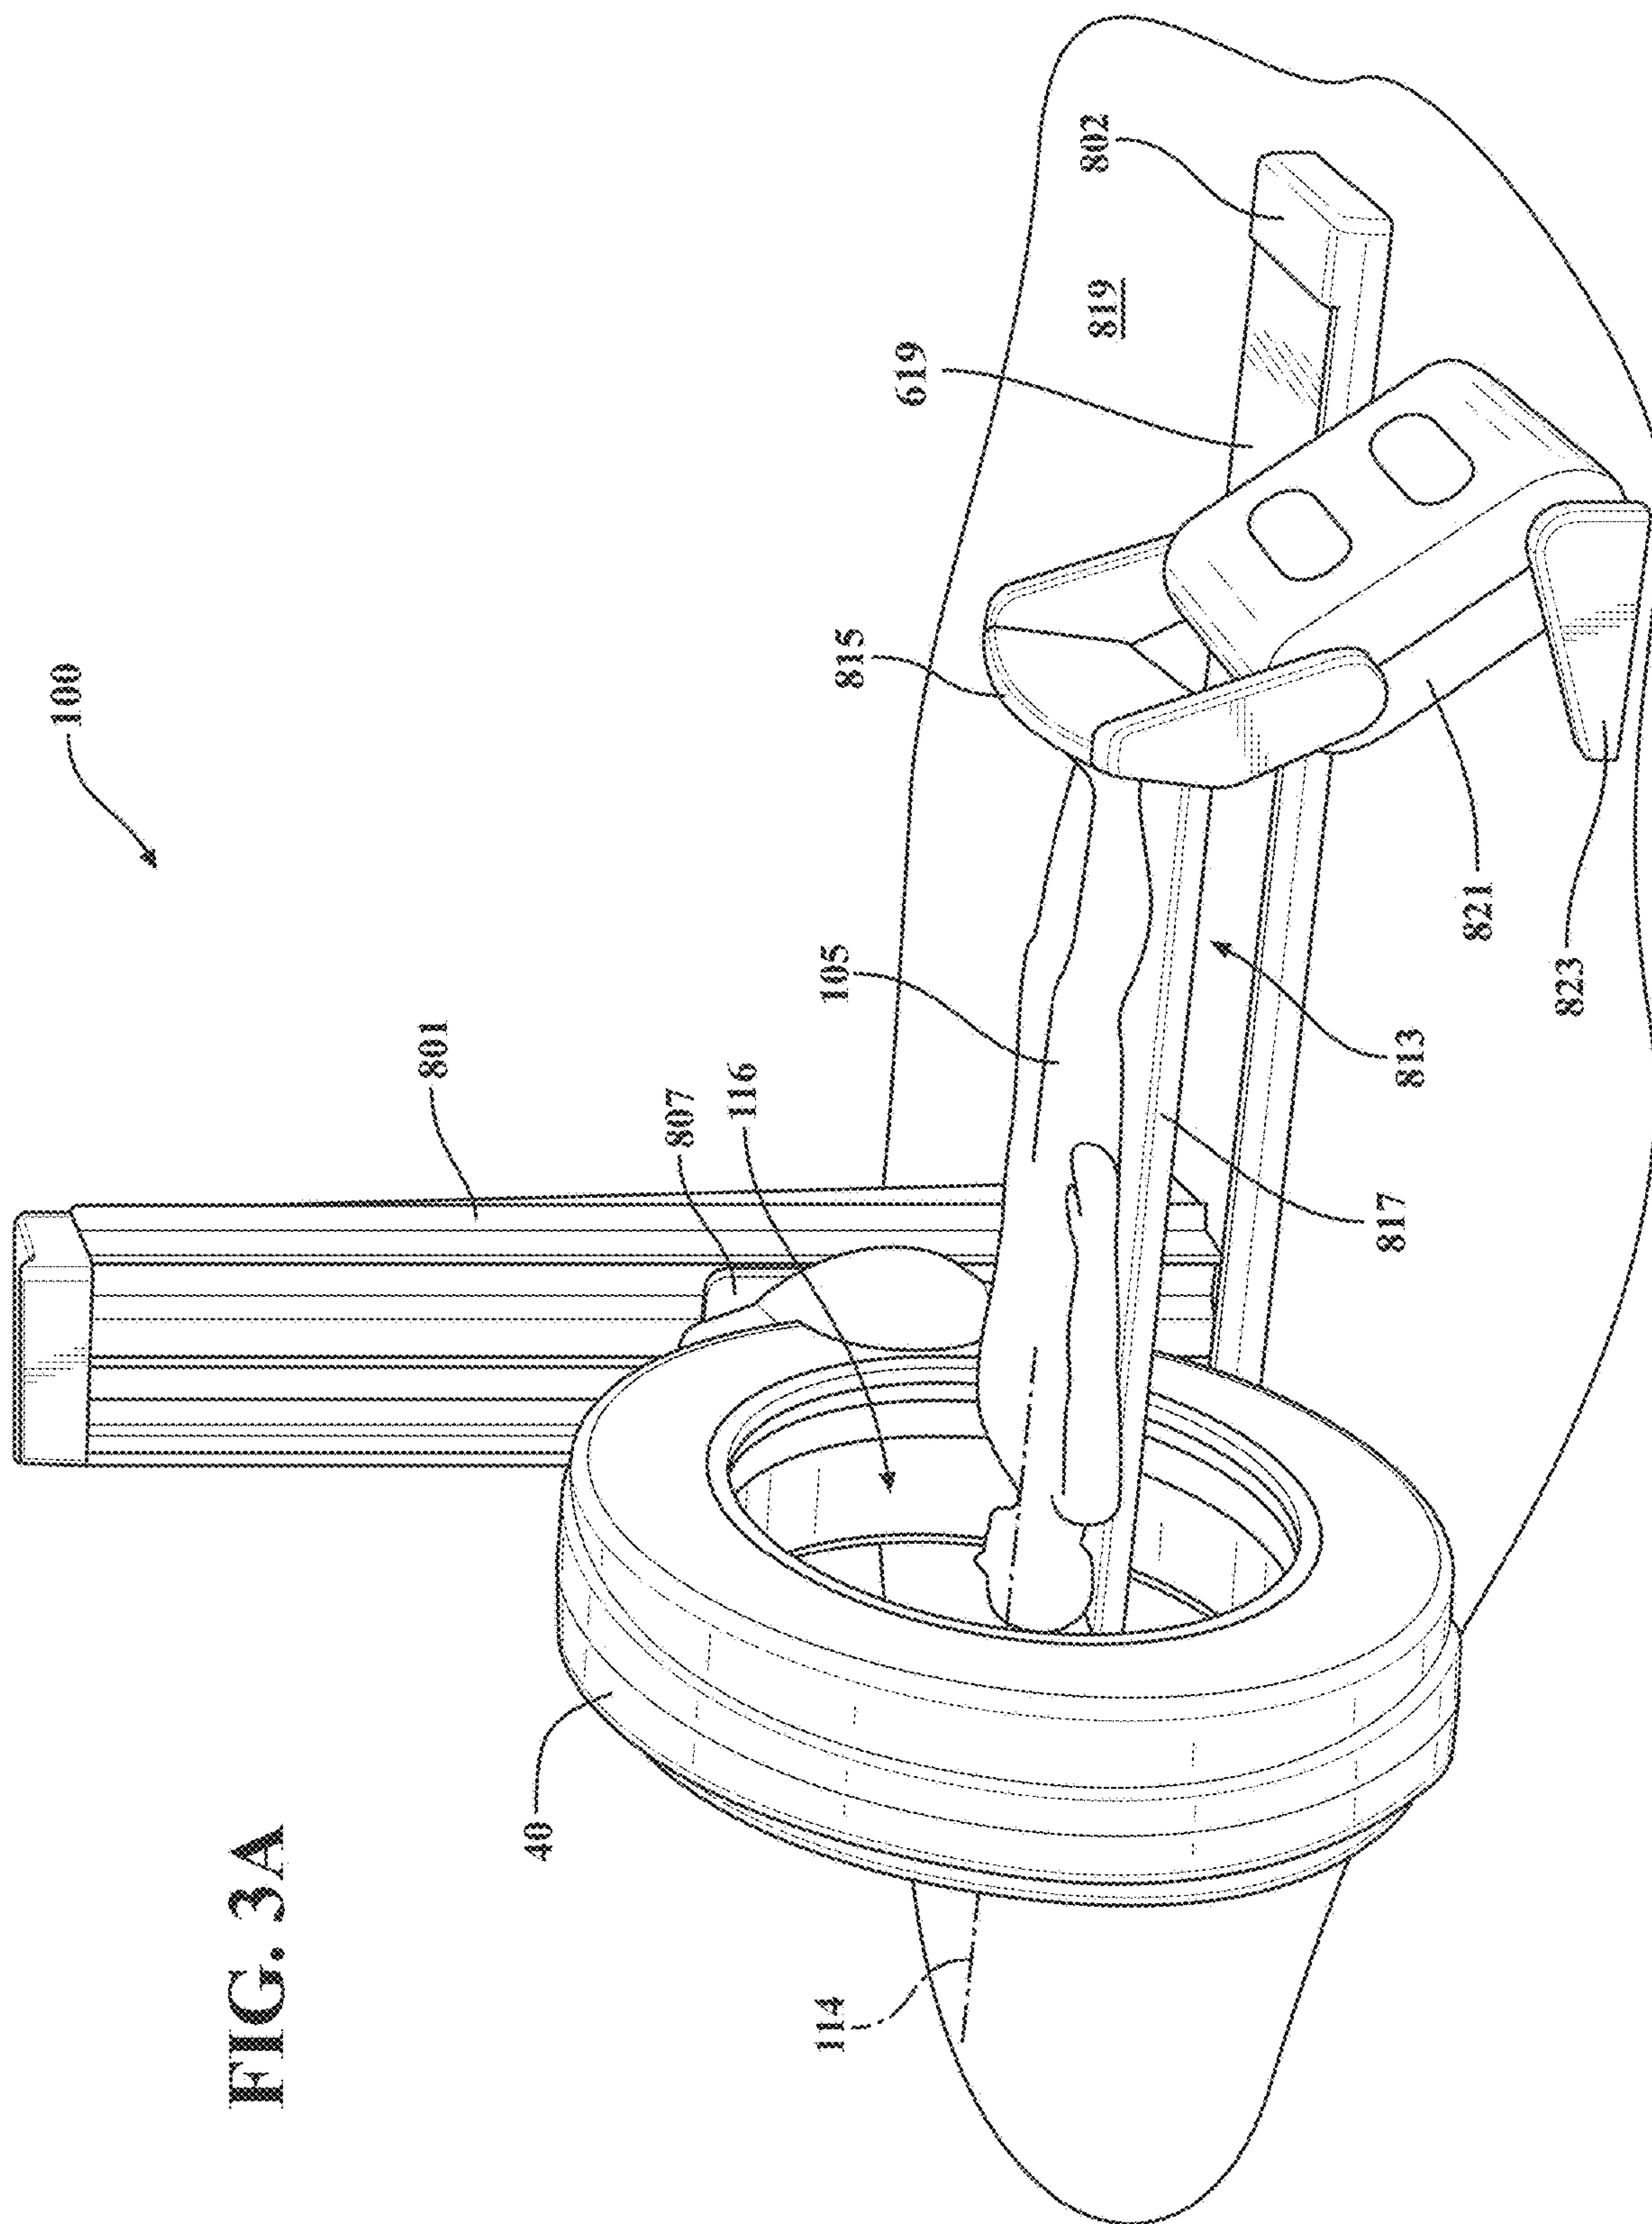


FIG. 3A

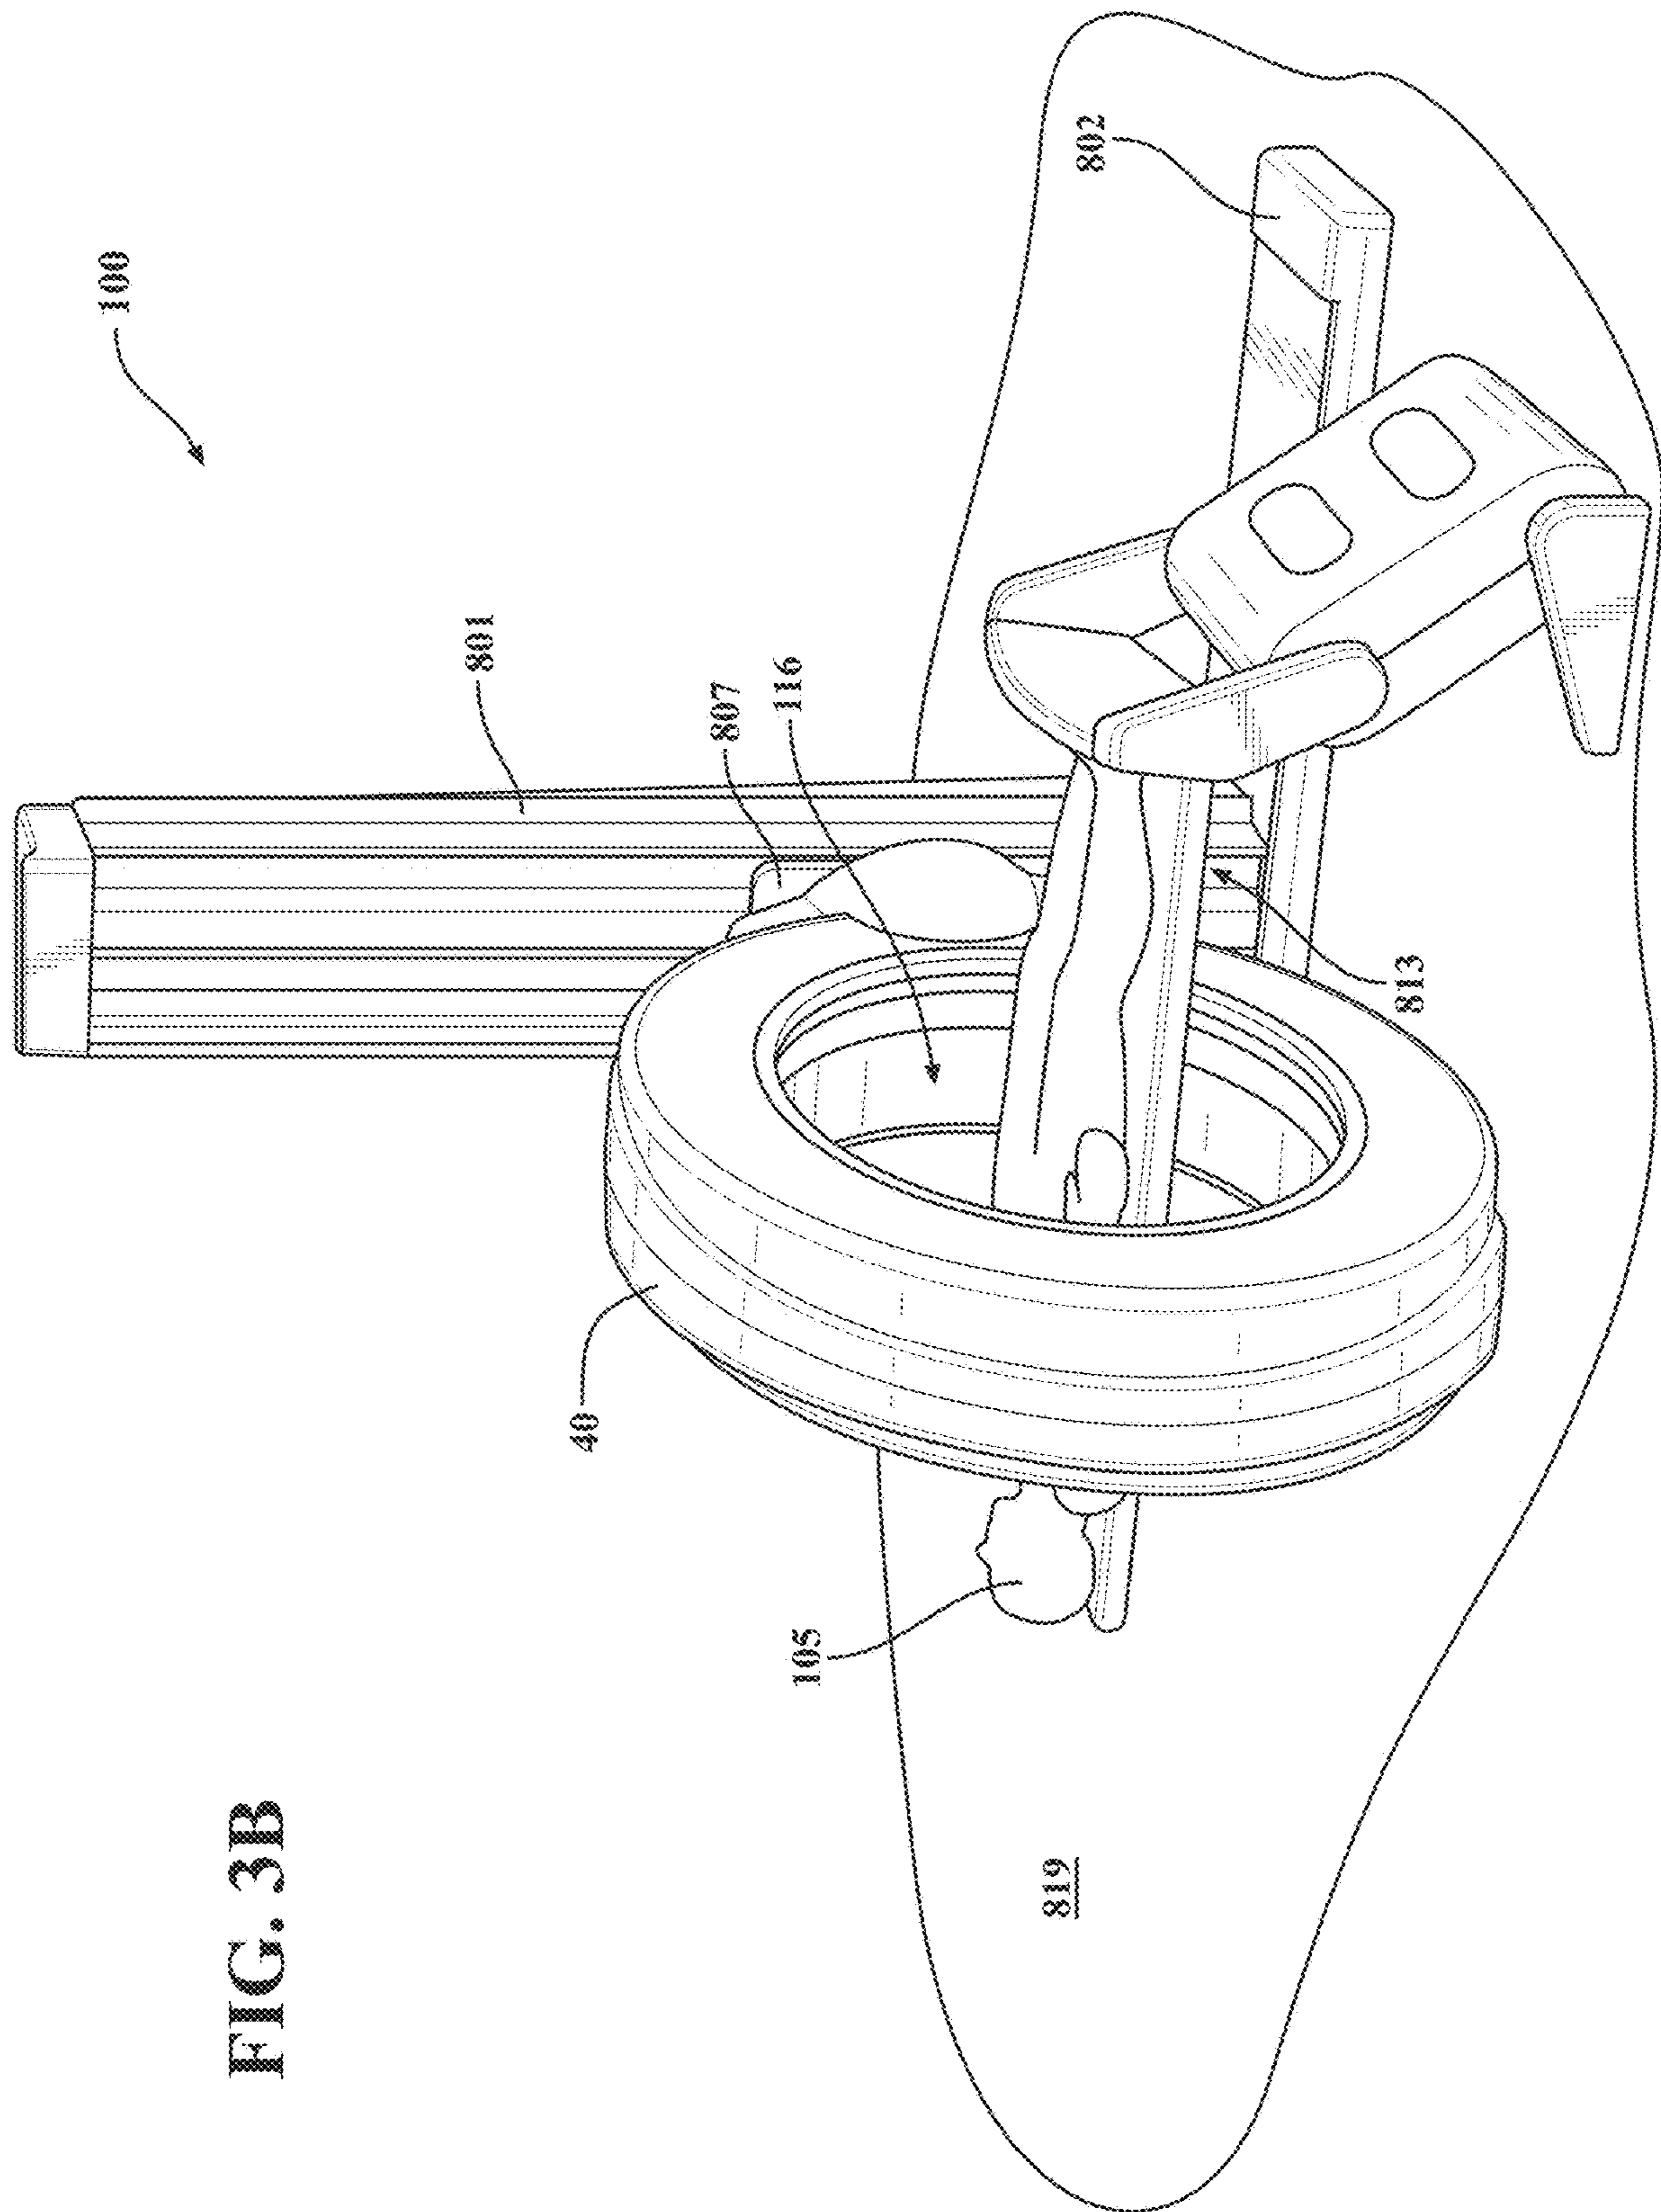


FIG. 3B

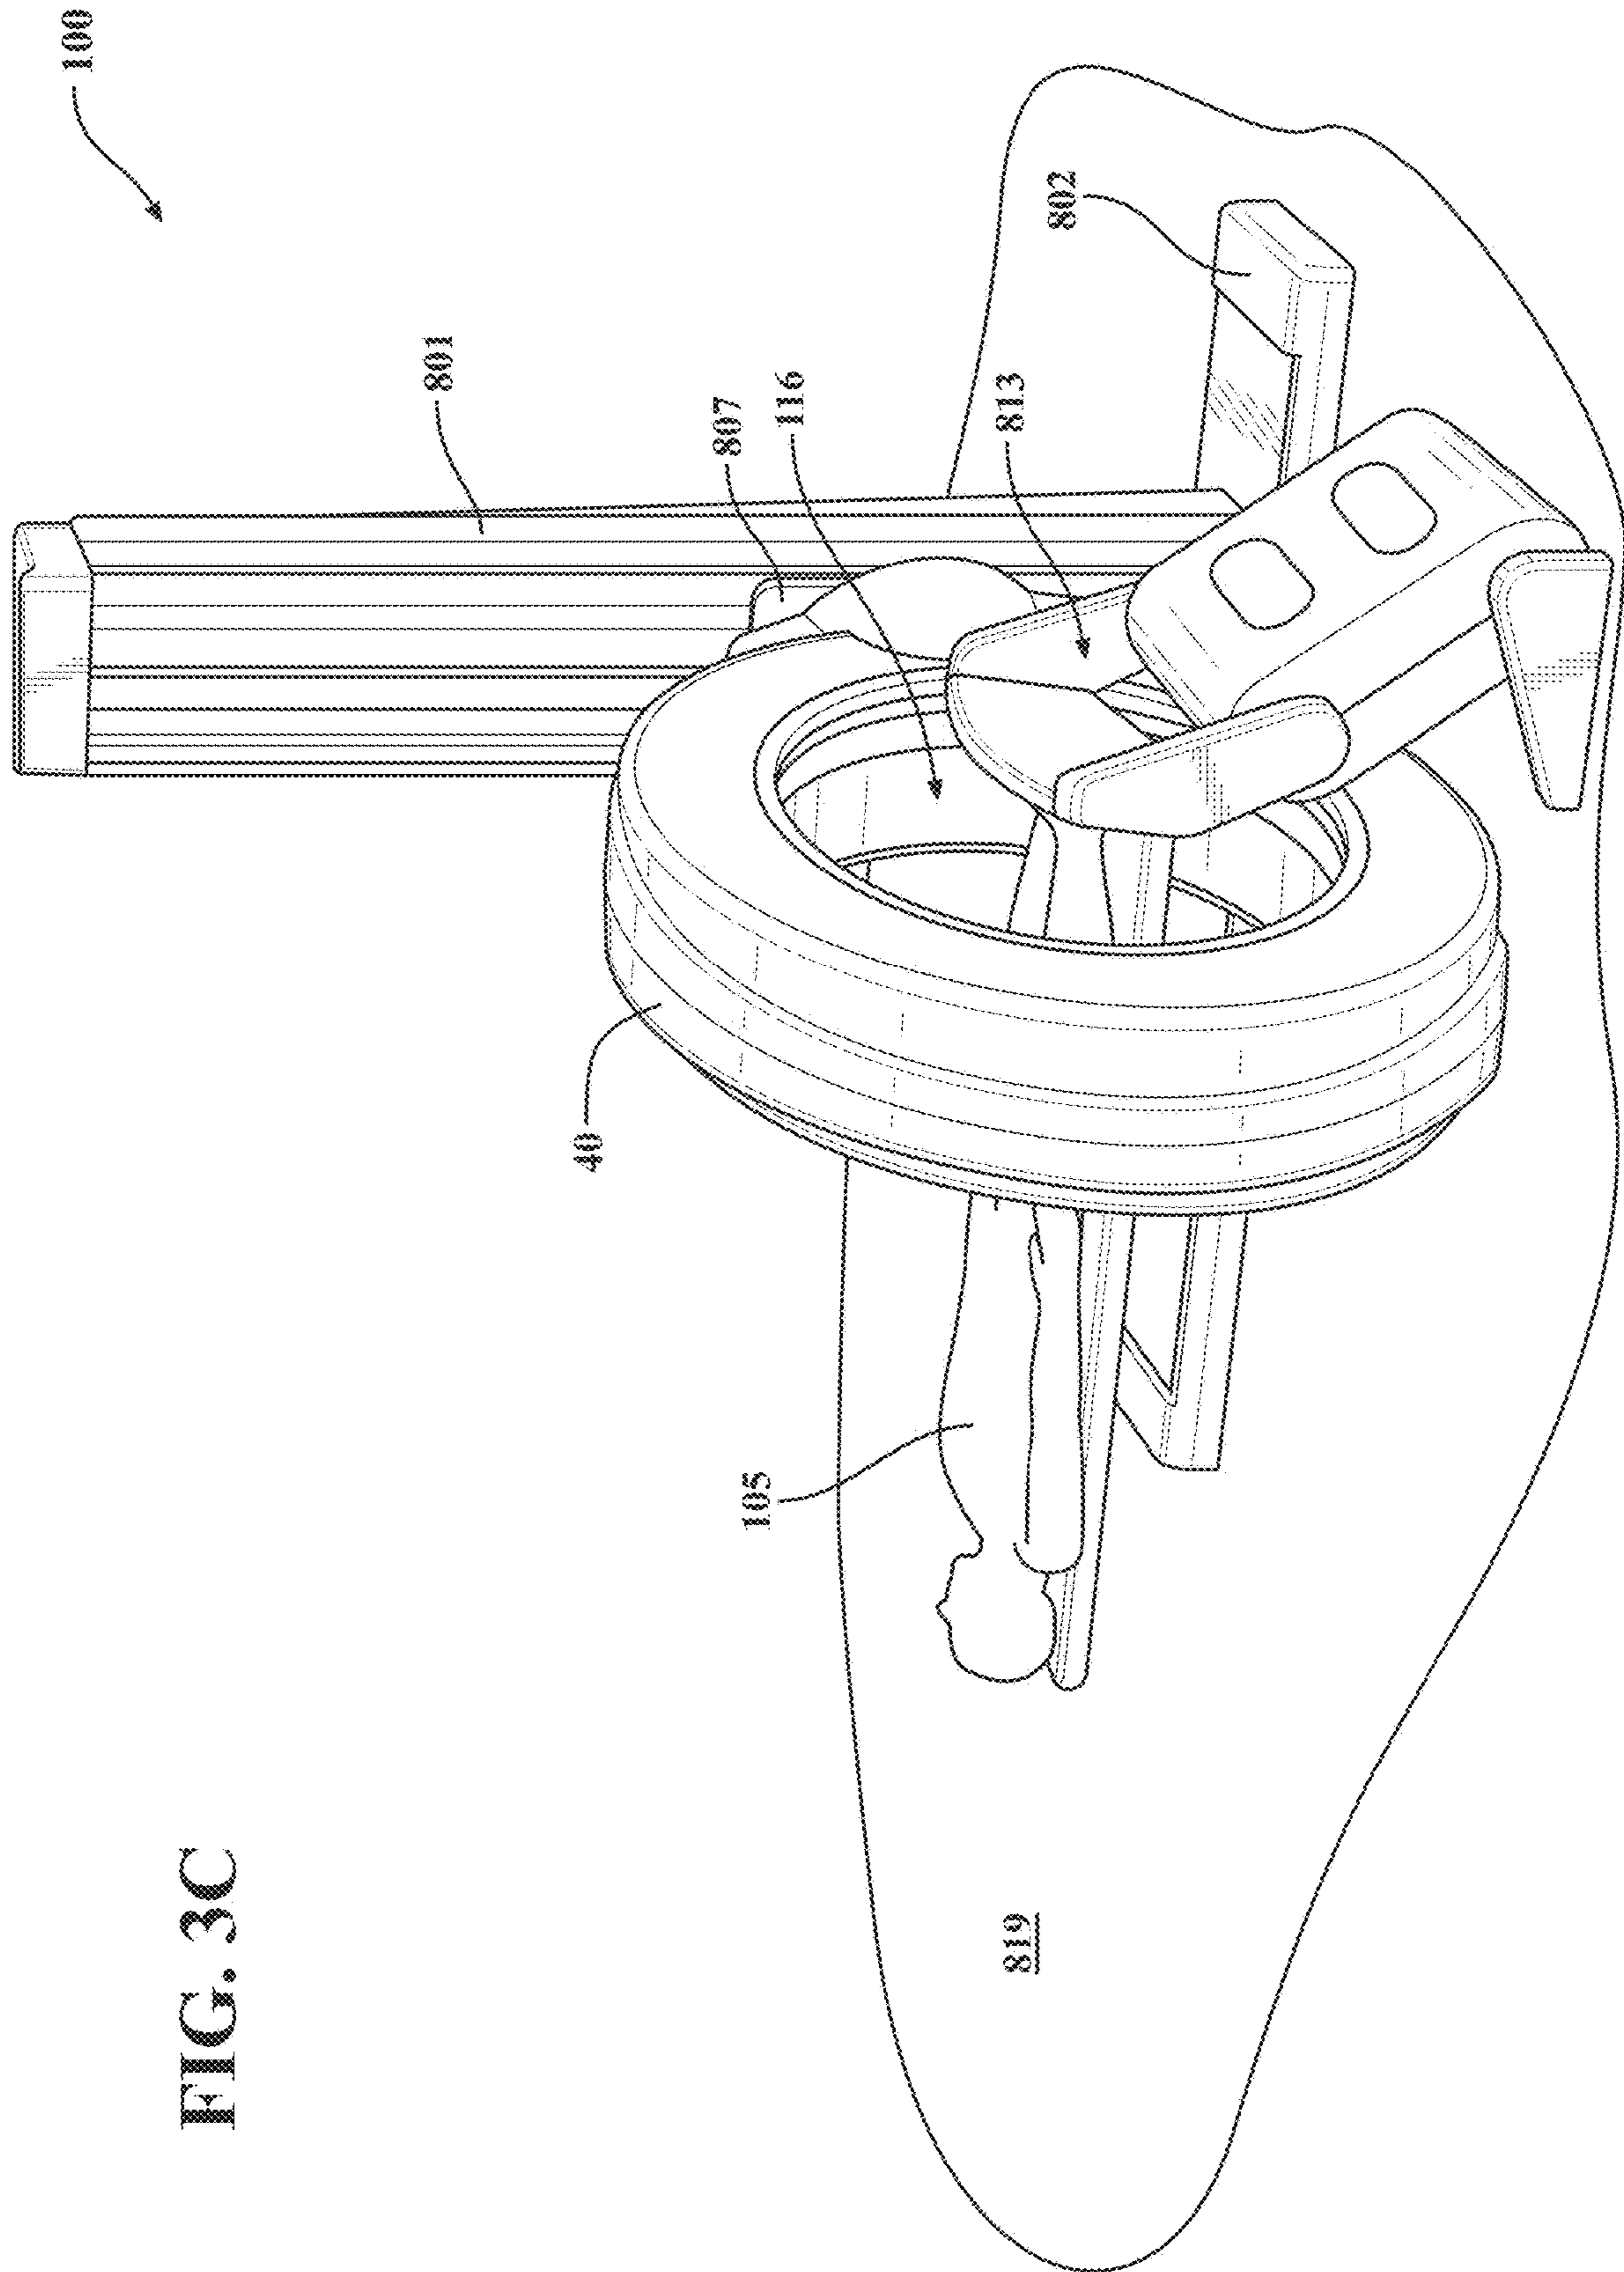


FIG. 3C

FIG. 4A

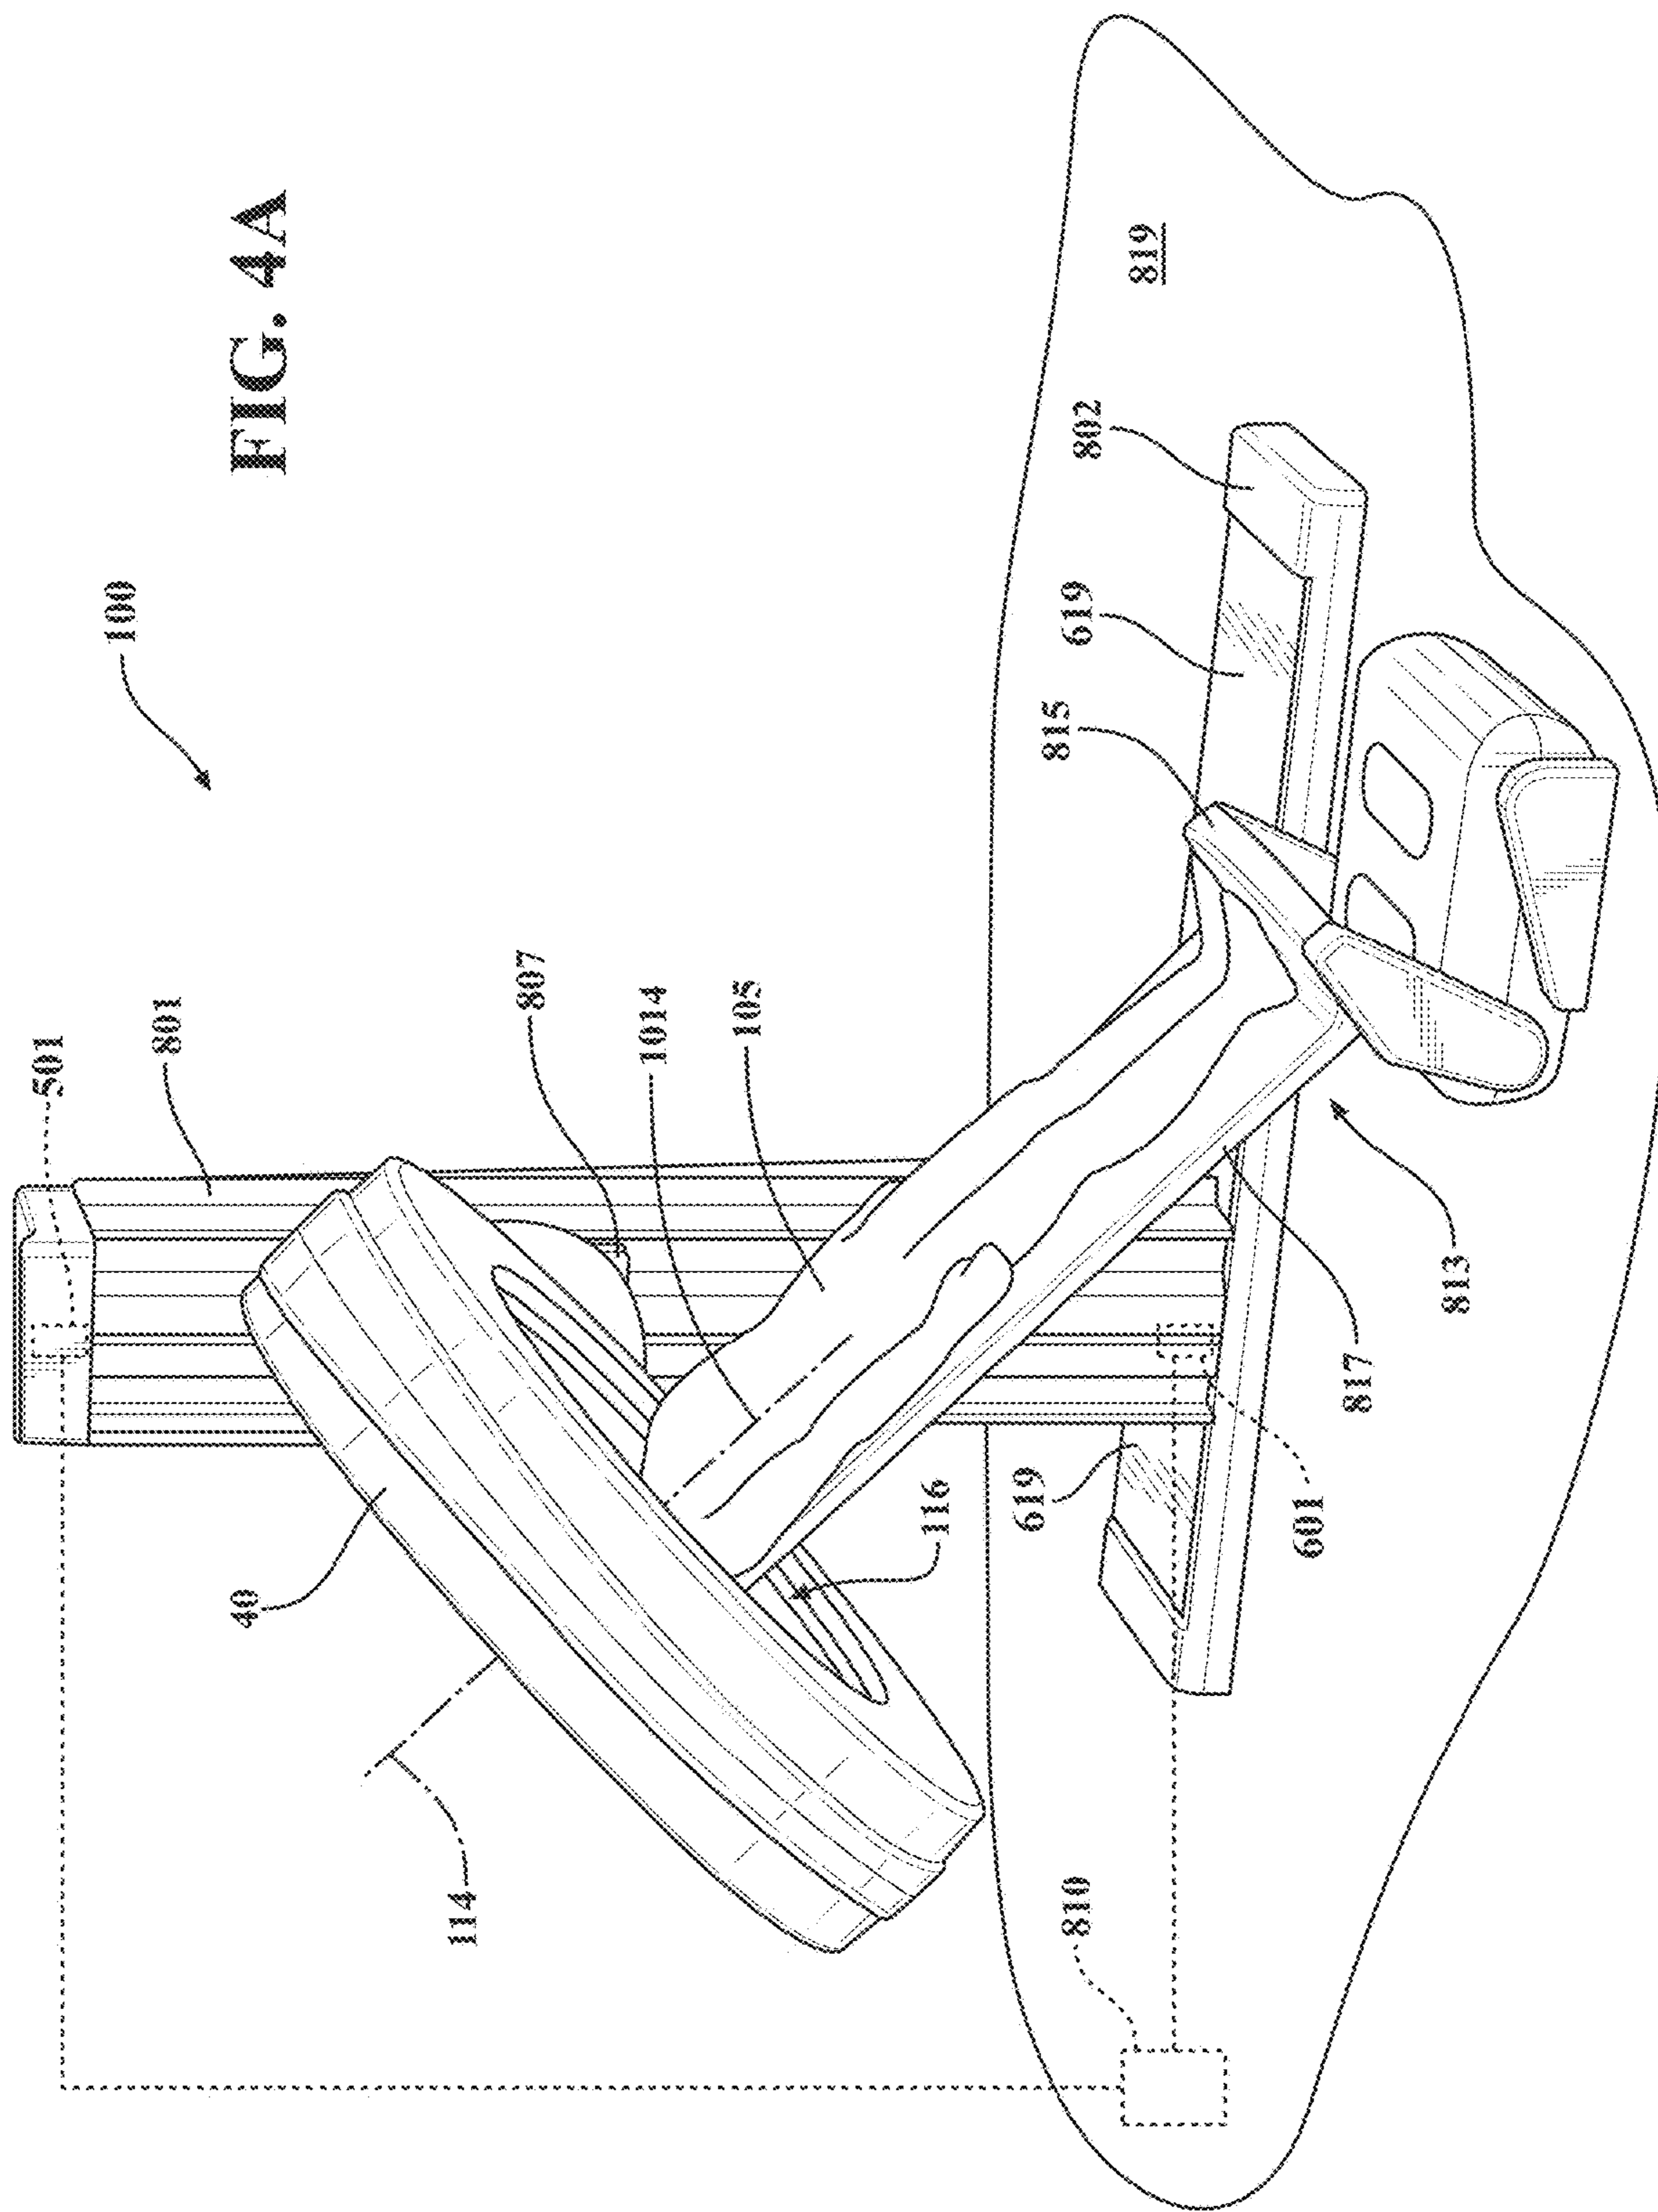


FIG. 4B

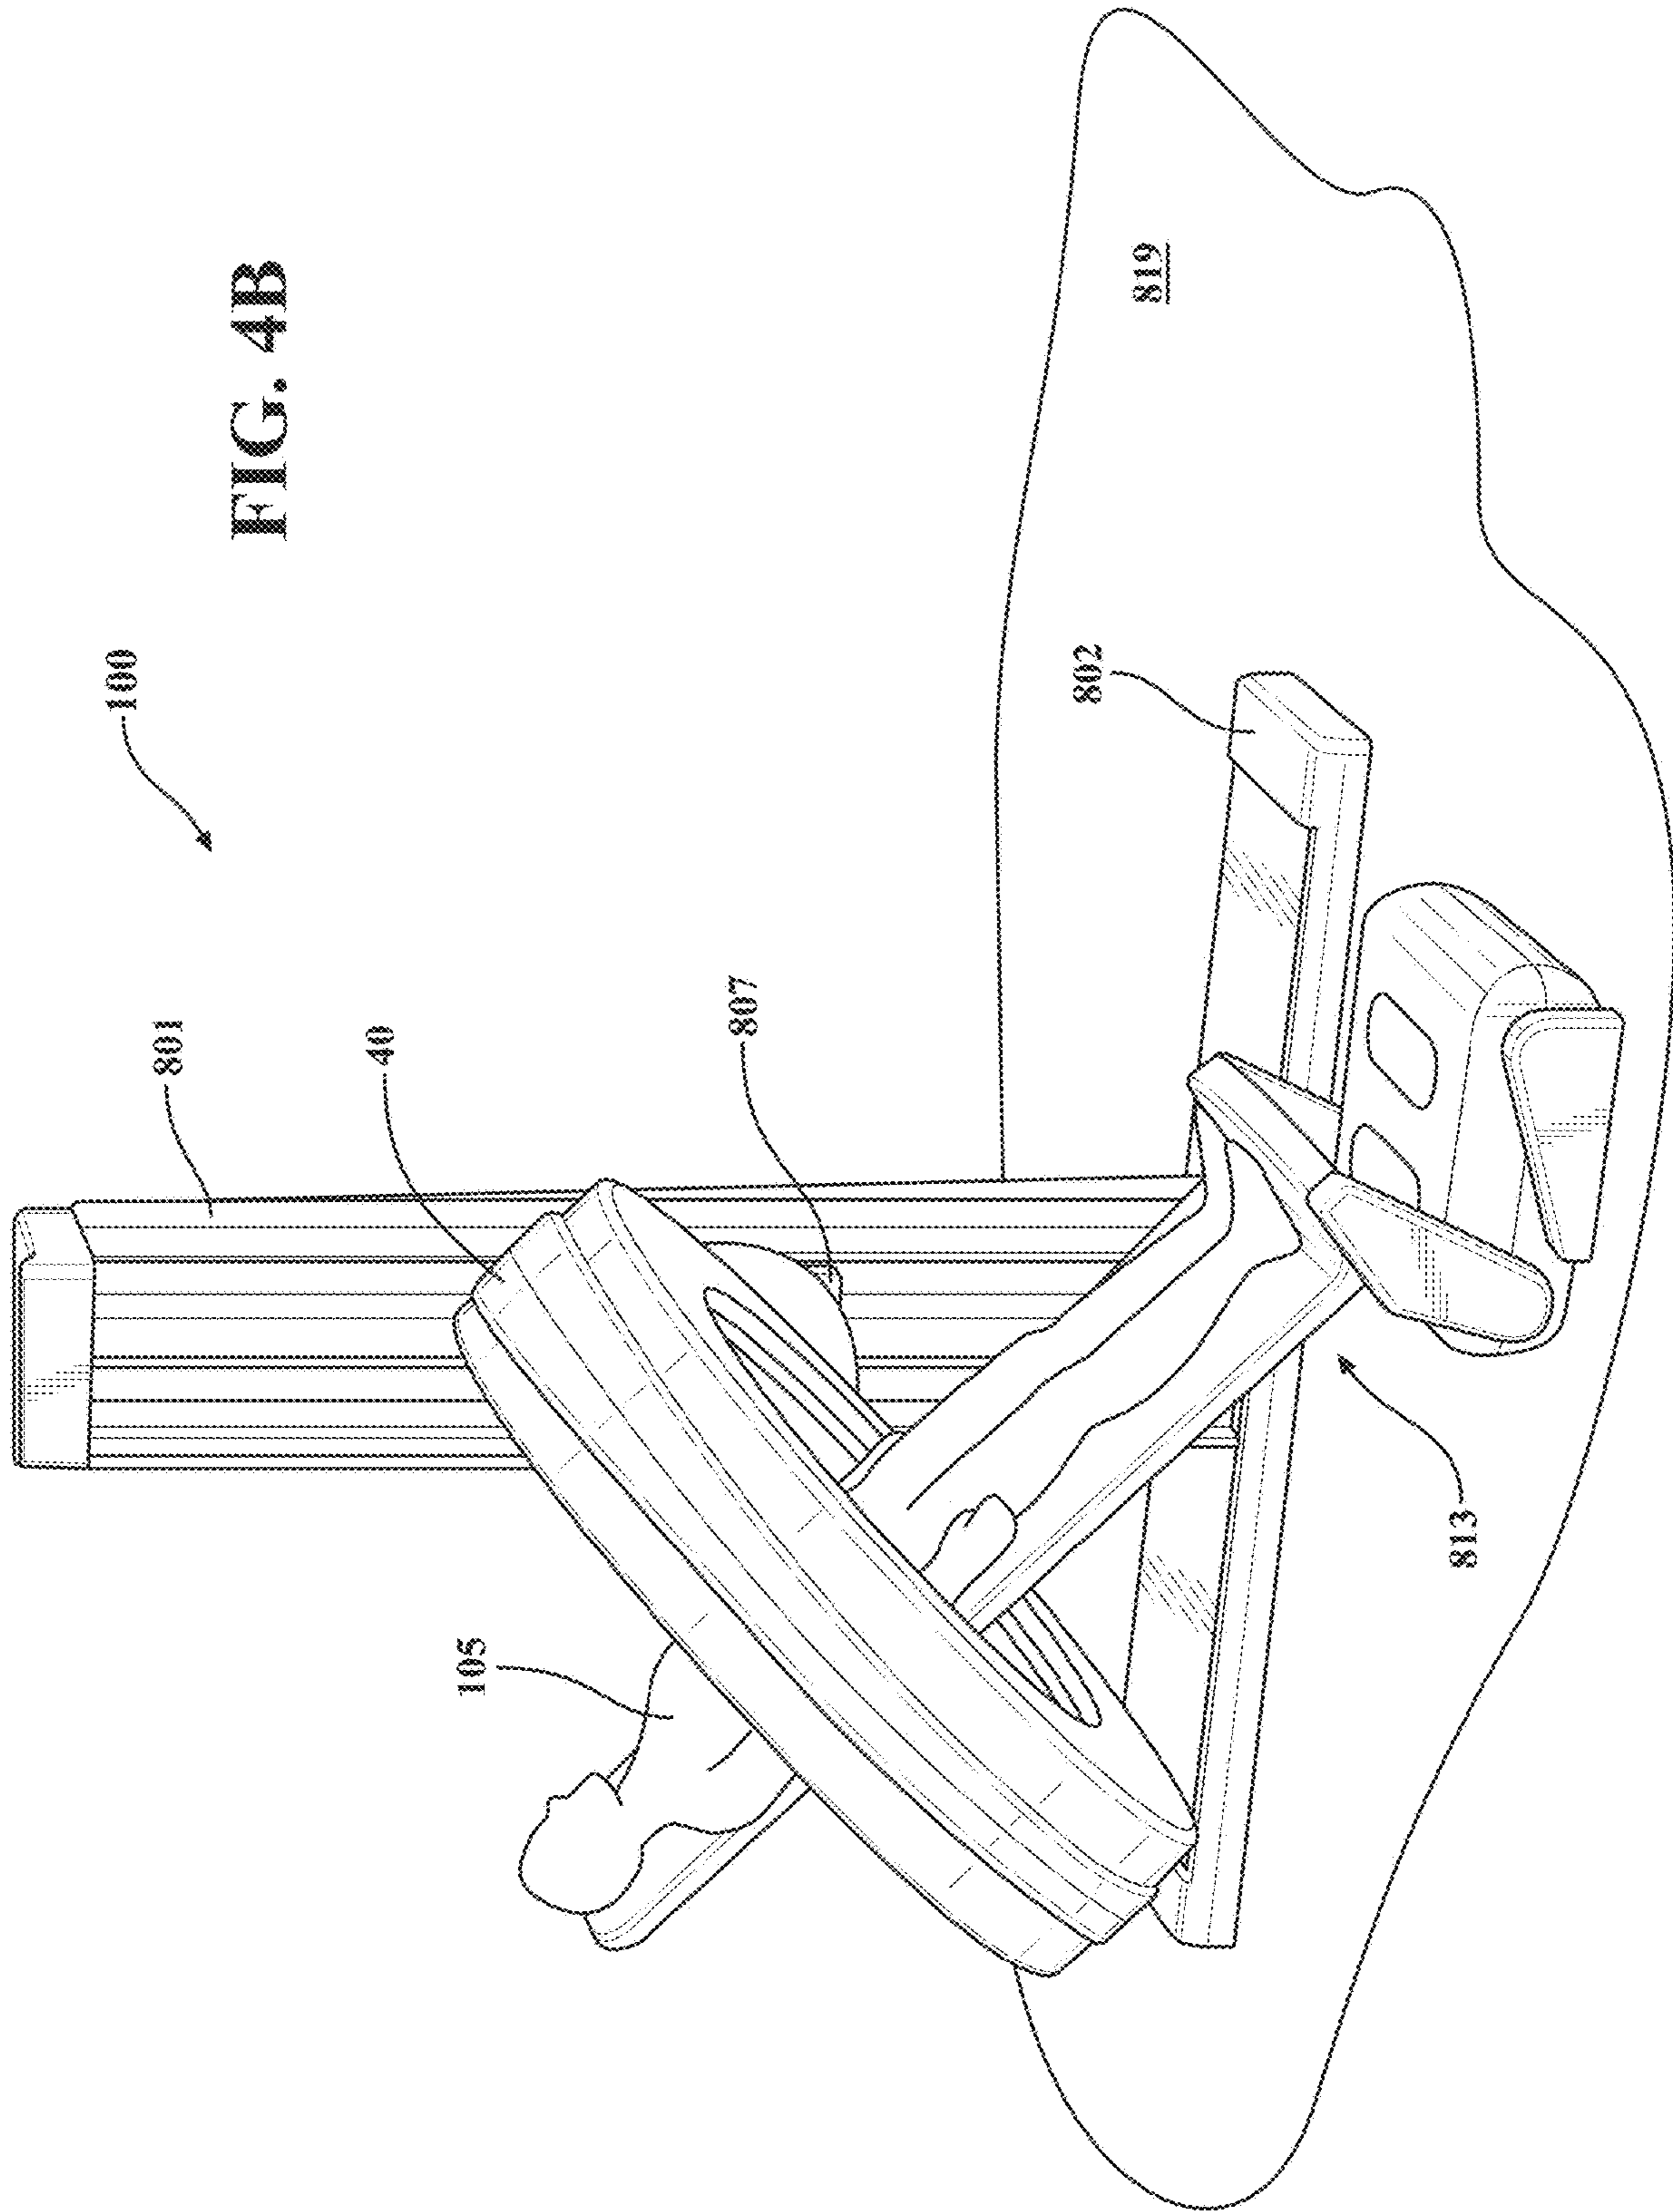
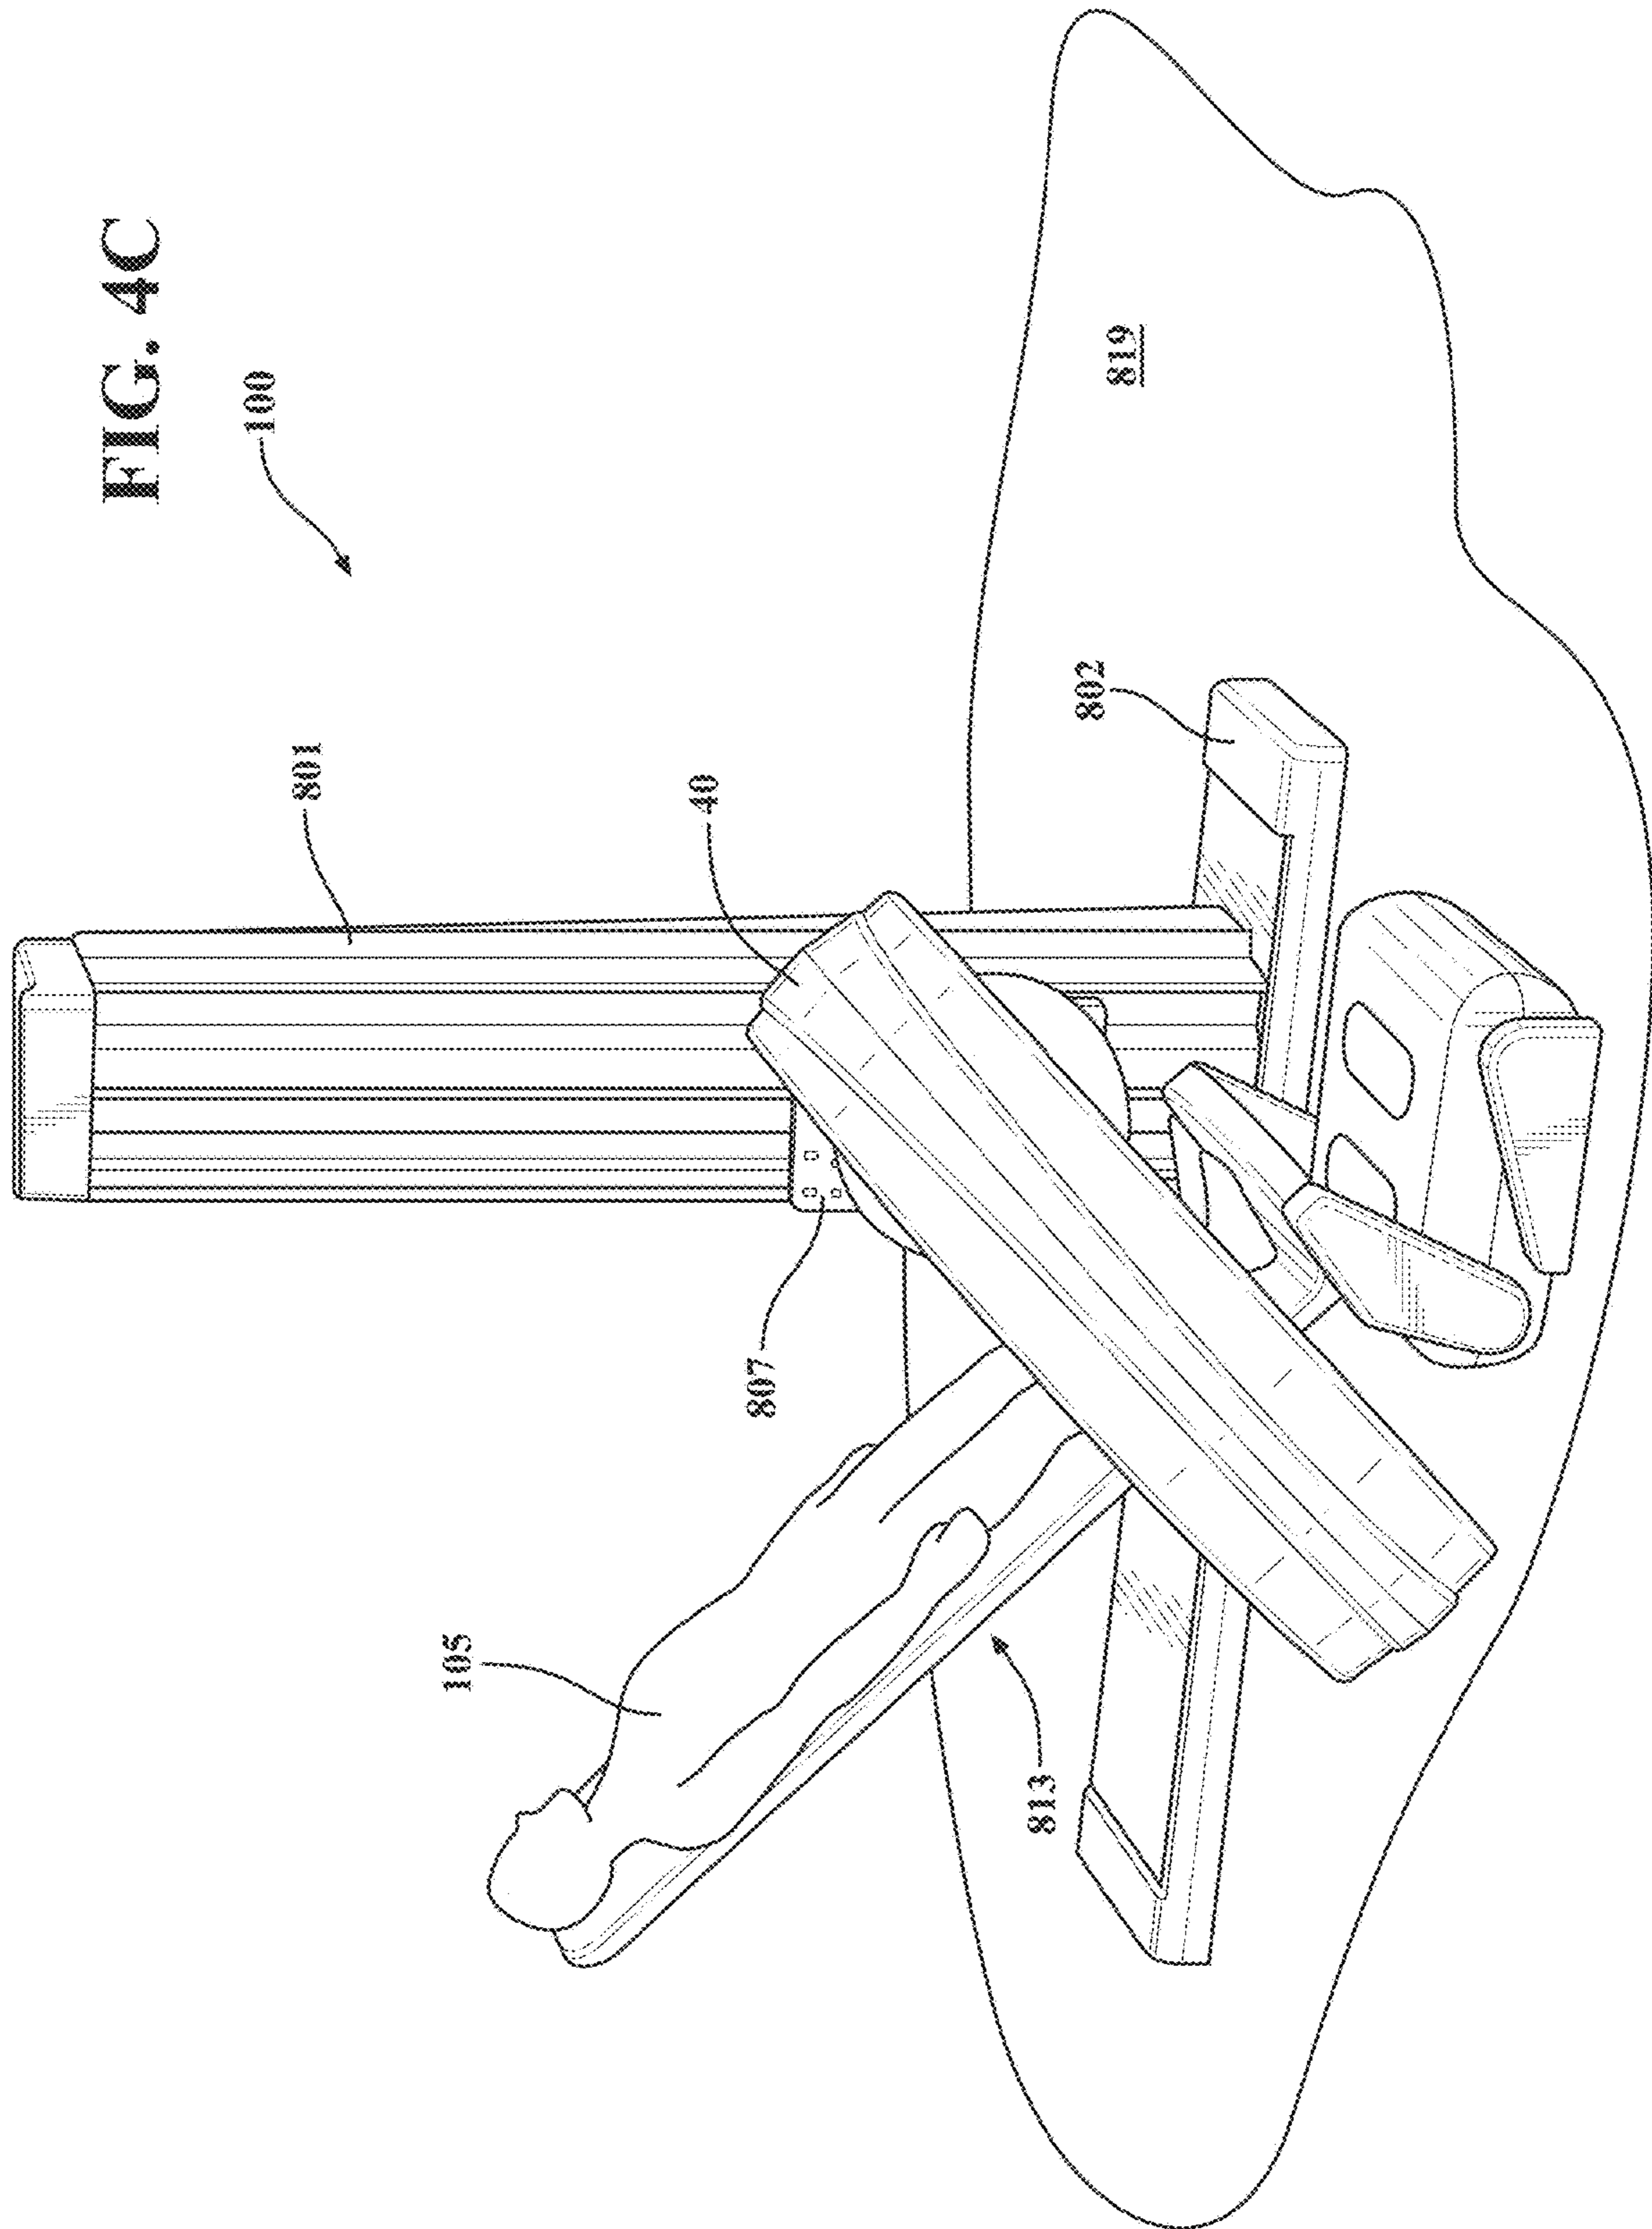


FIG. 4C



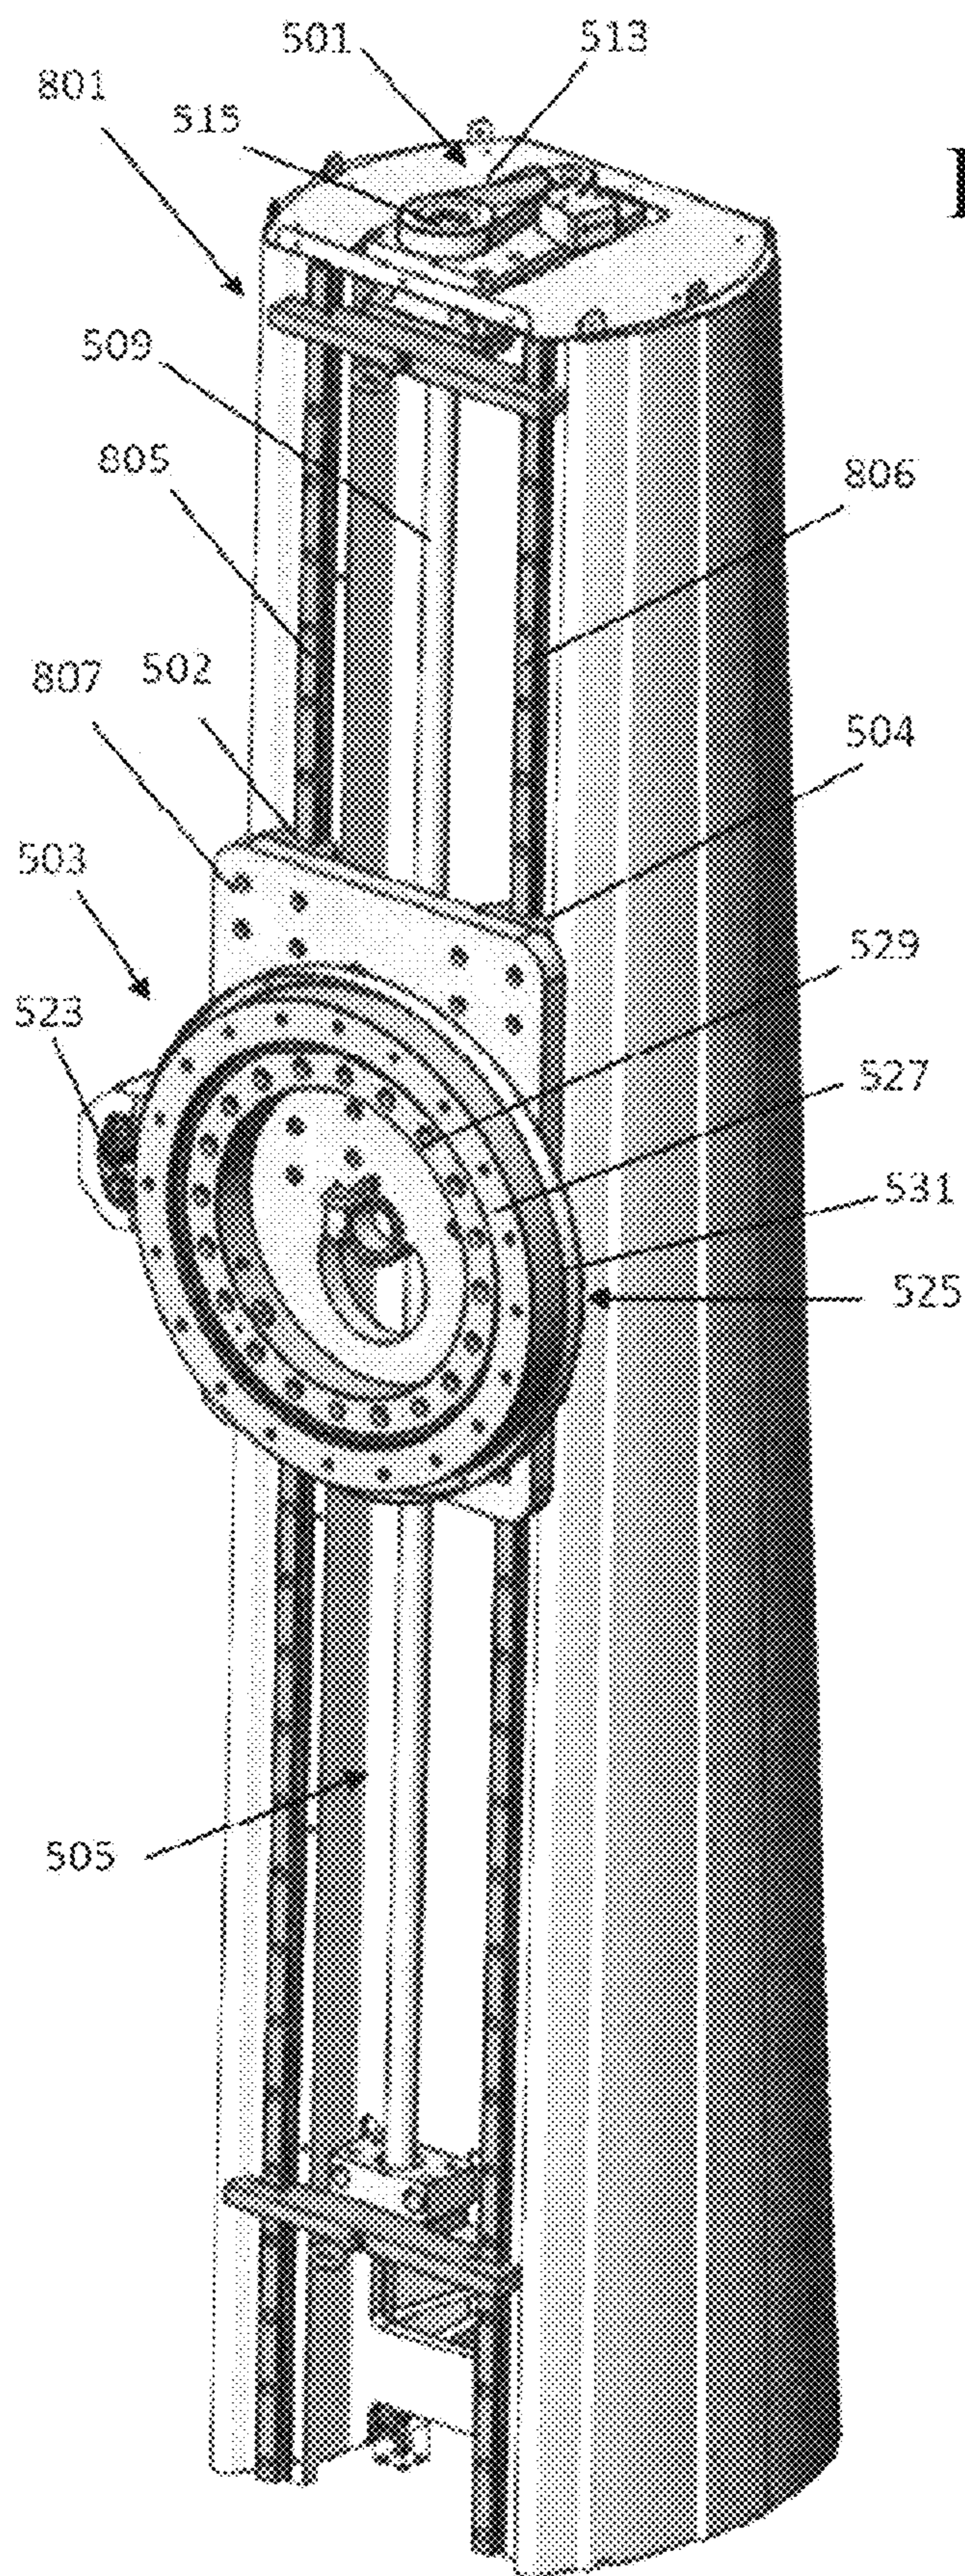


FIG. 5A

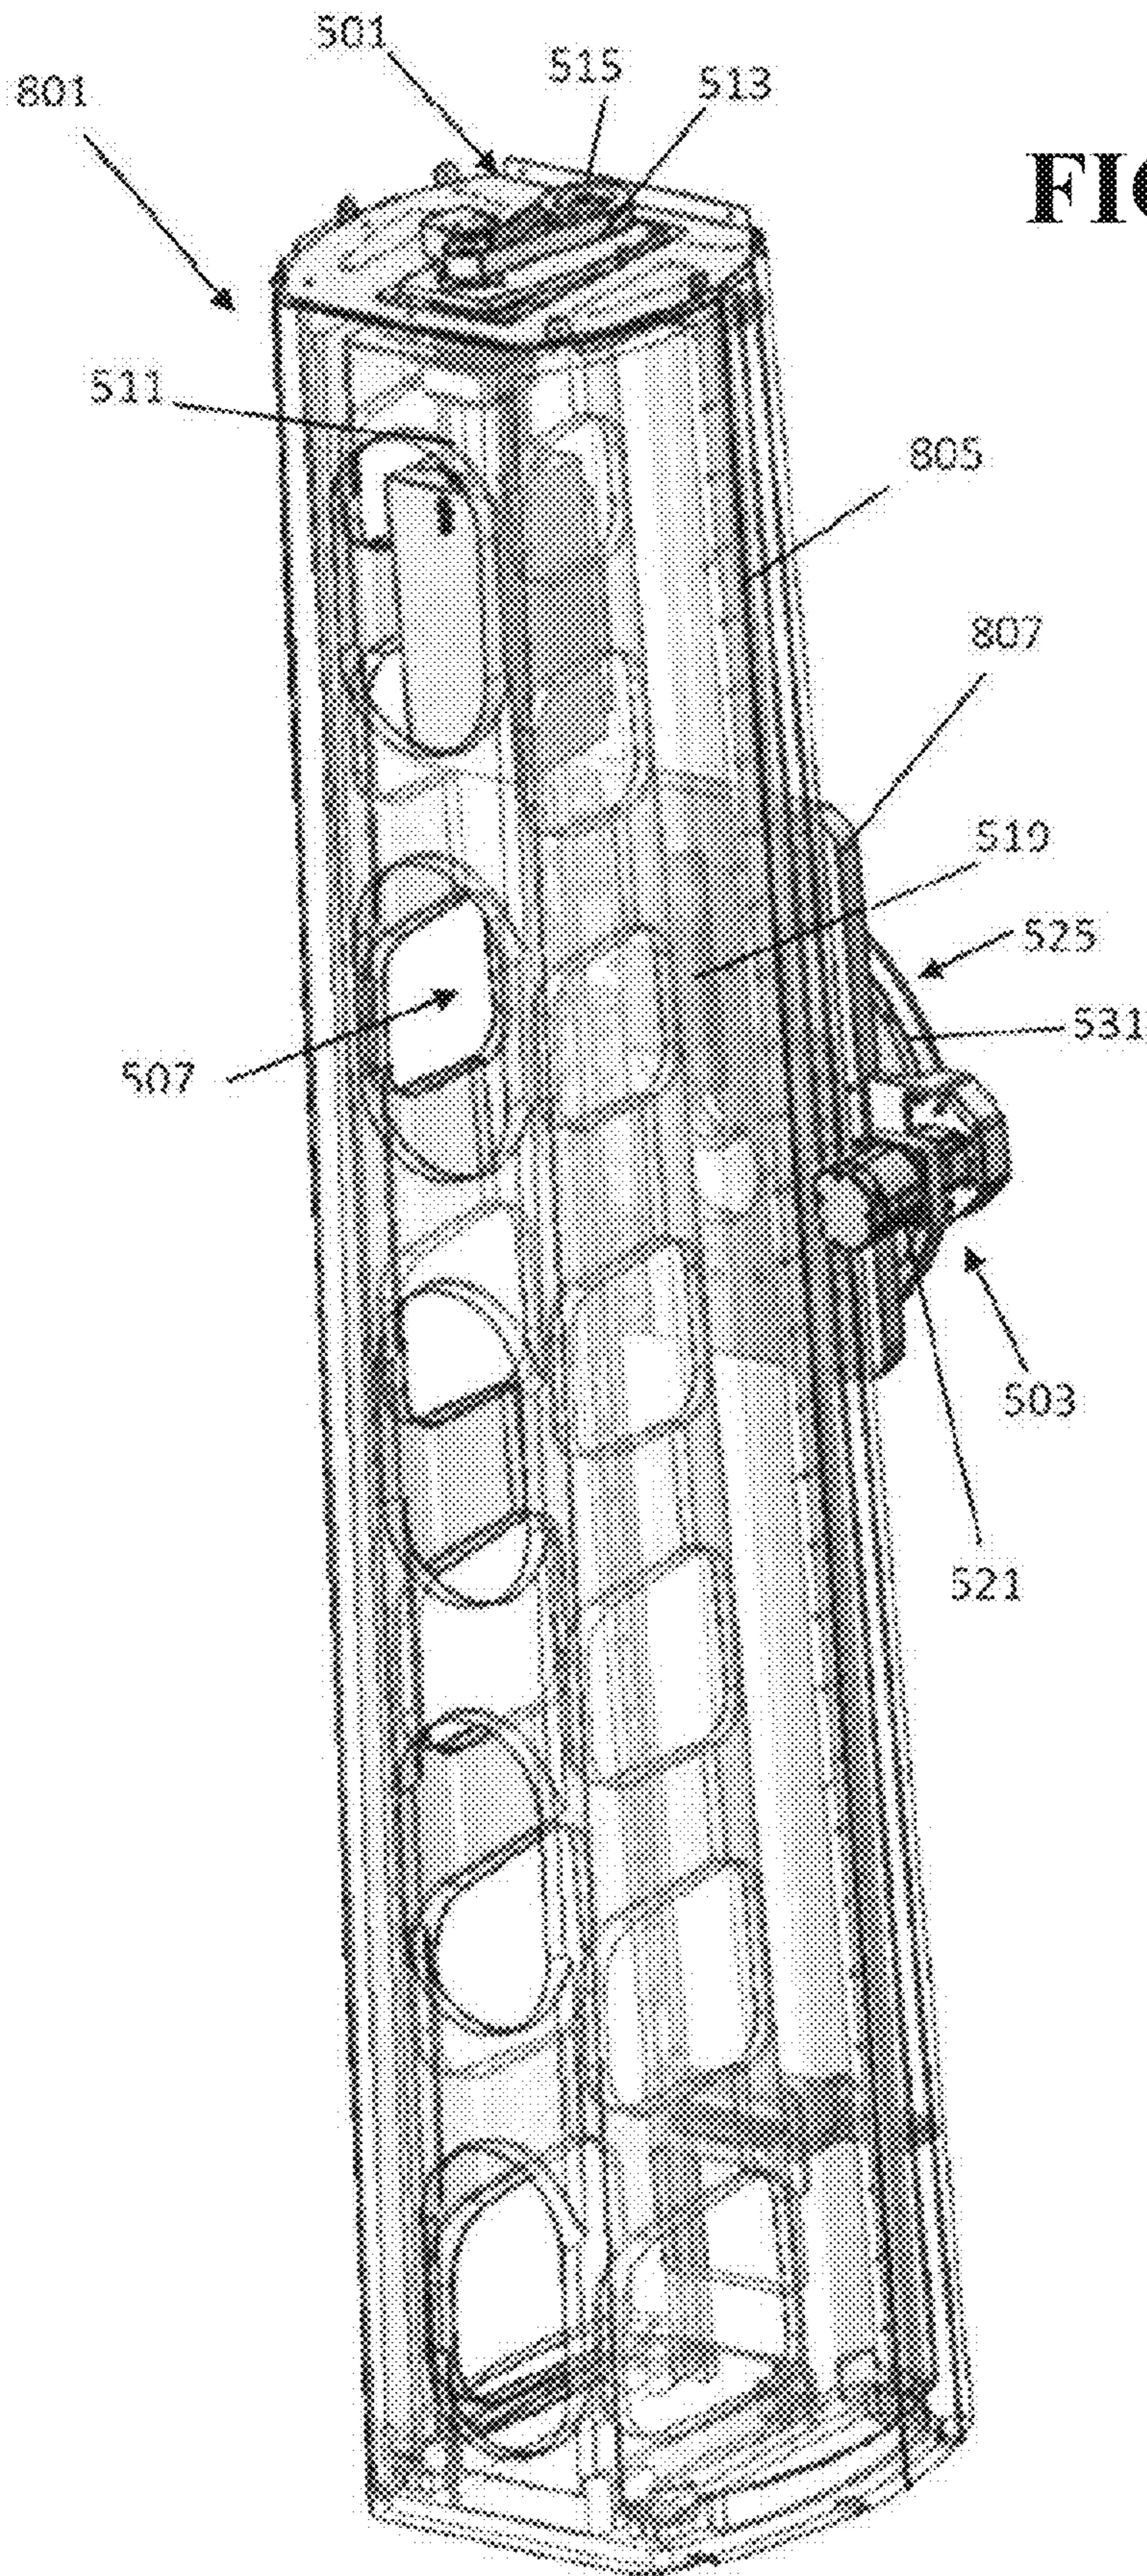


FIG. 5B

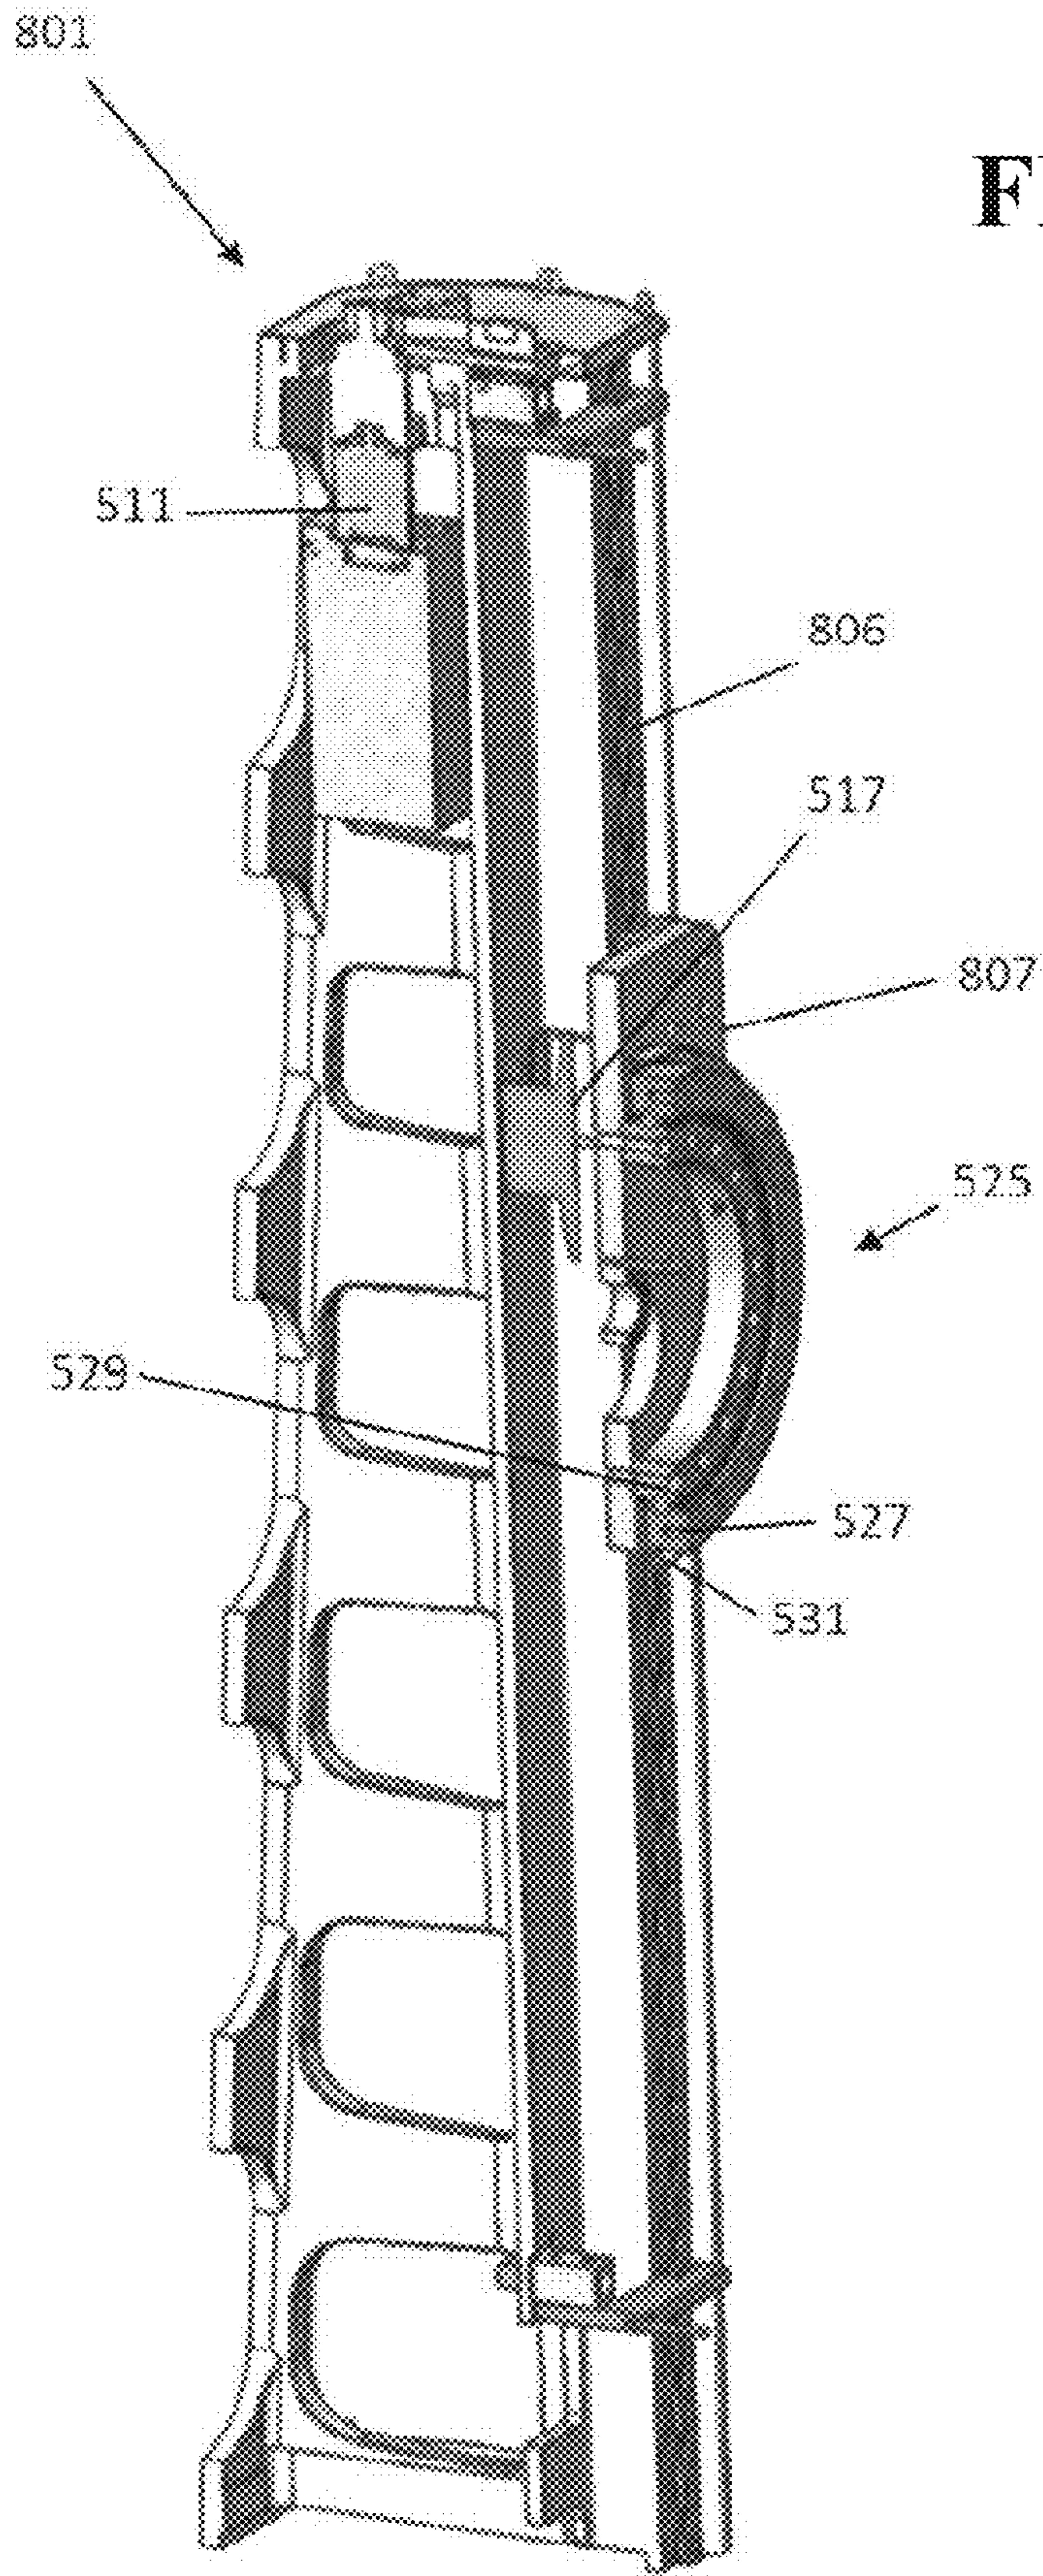
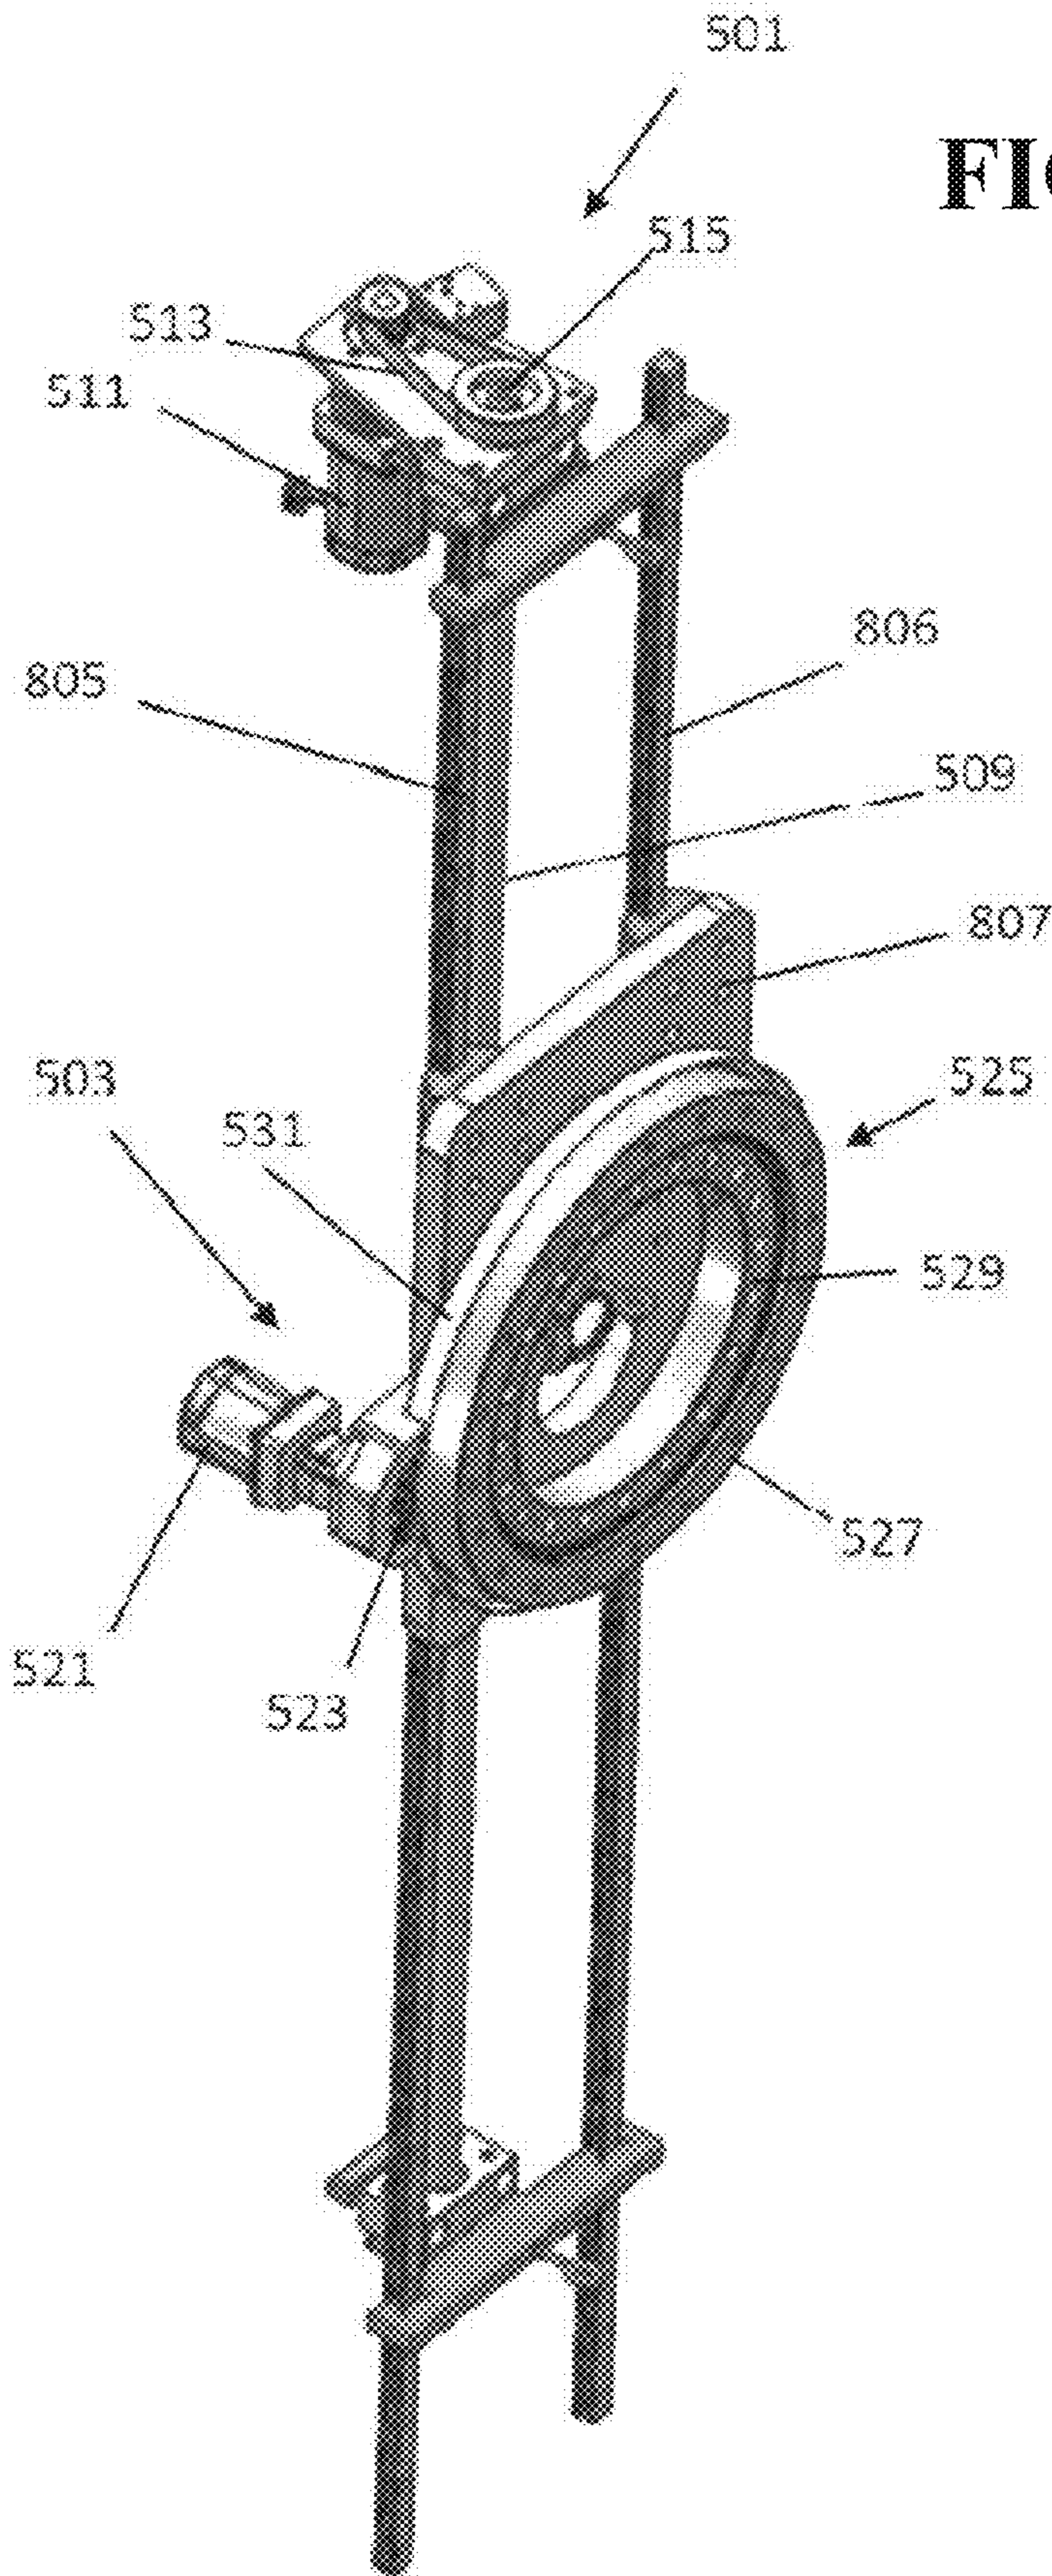


FIG. 5C

FIG. 5D



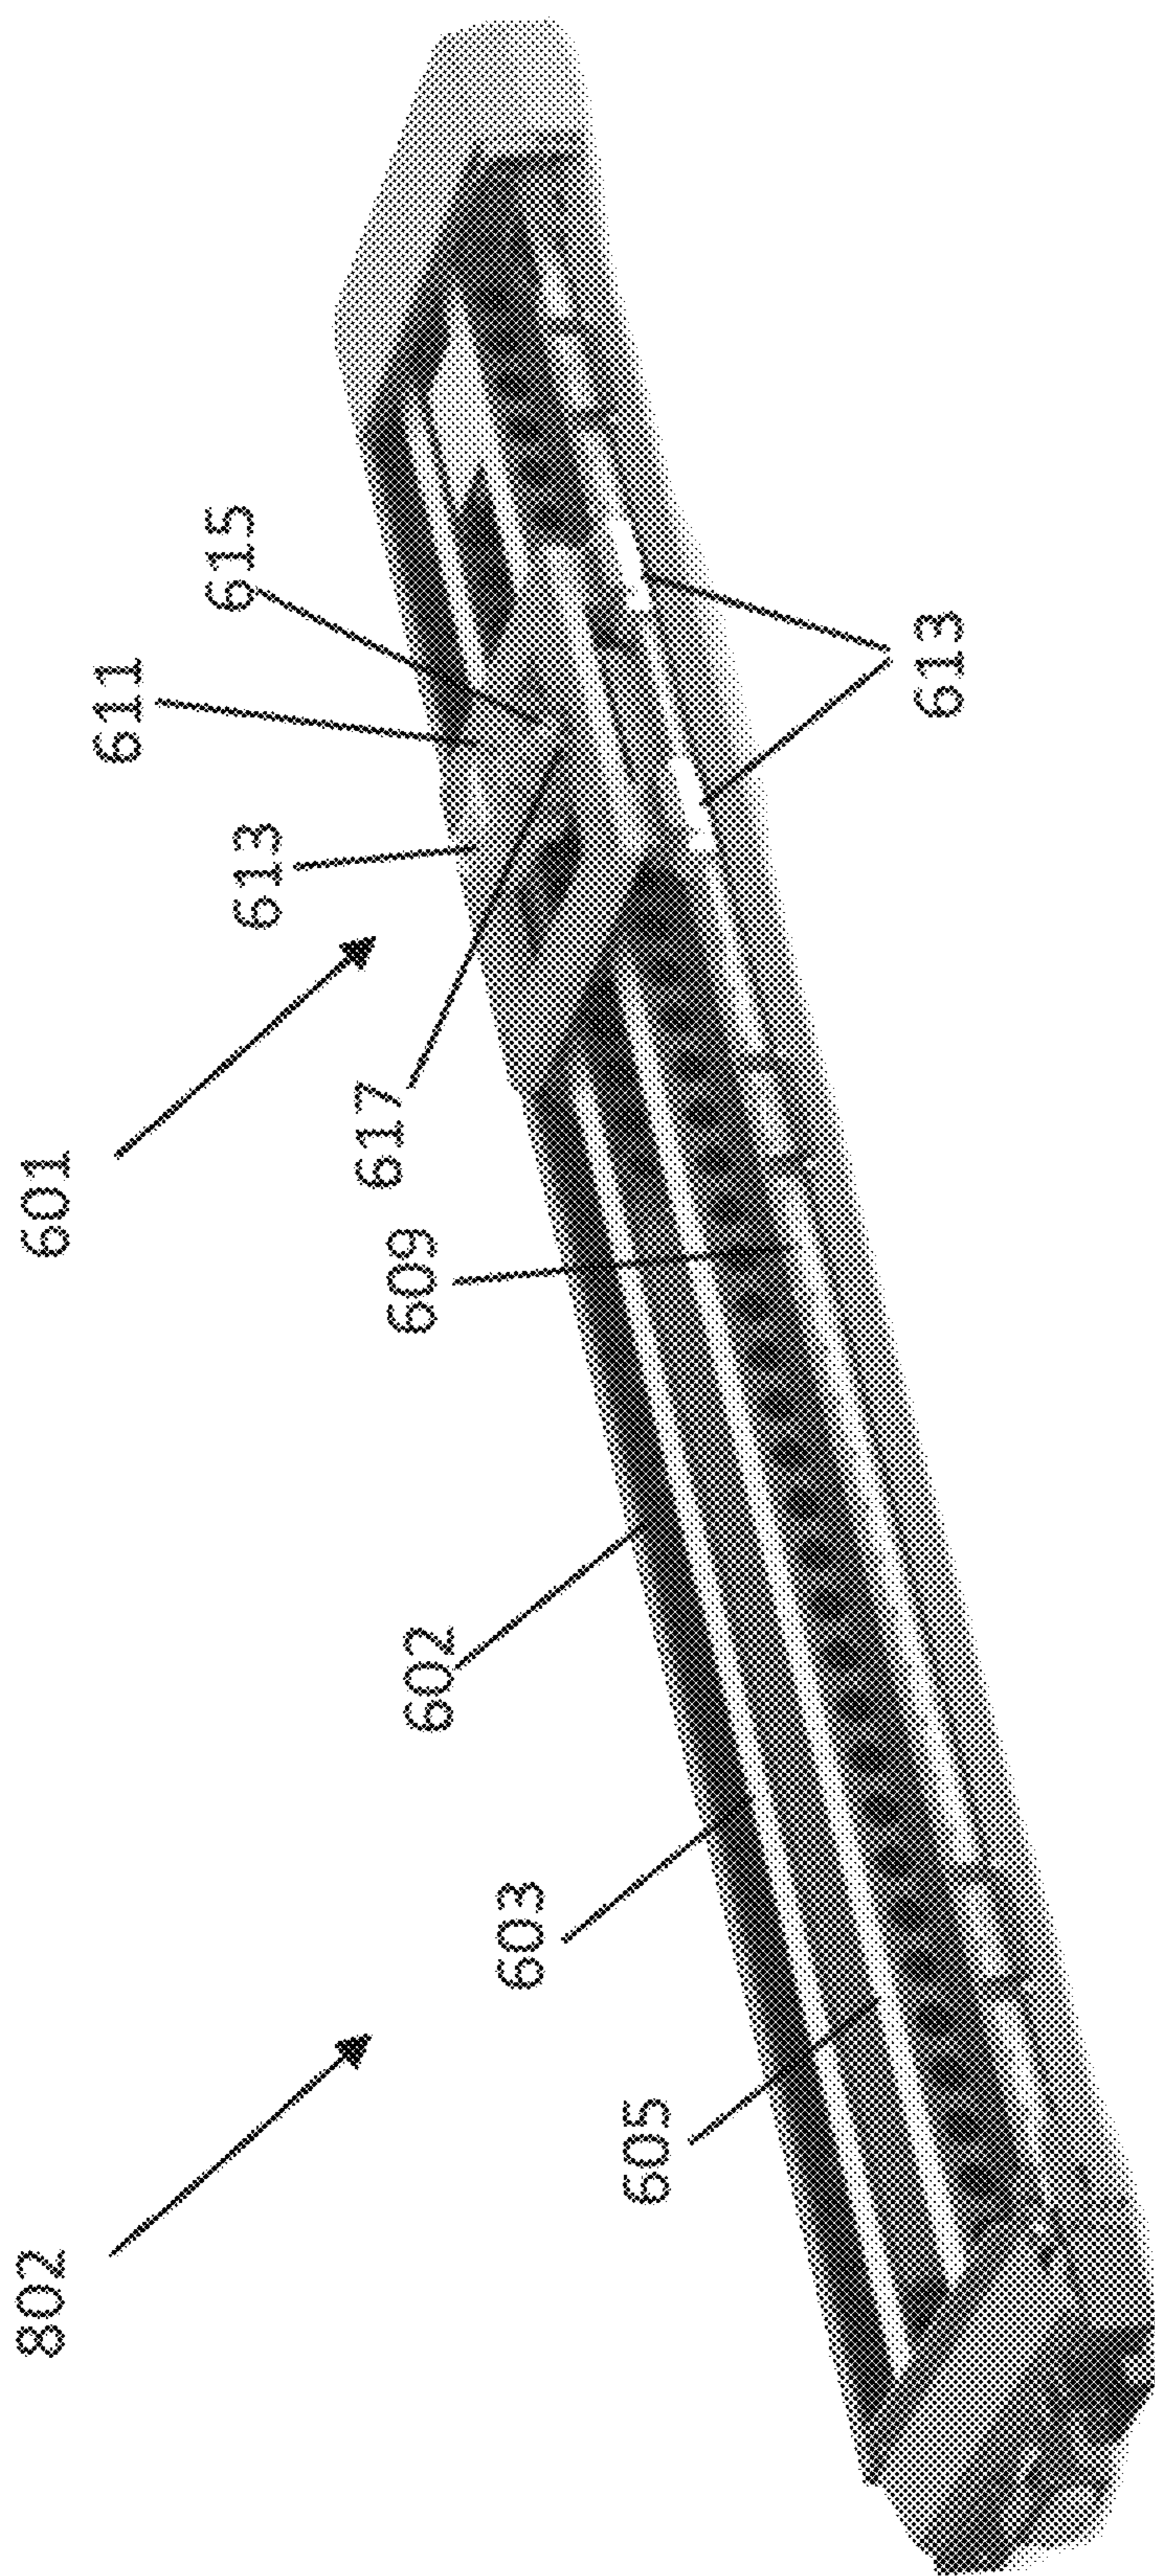


FIG. 6A

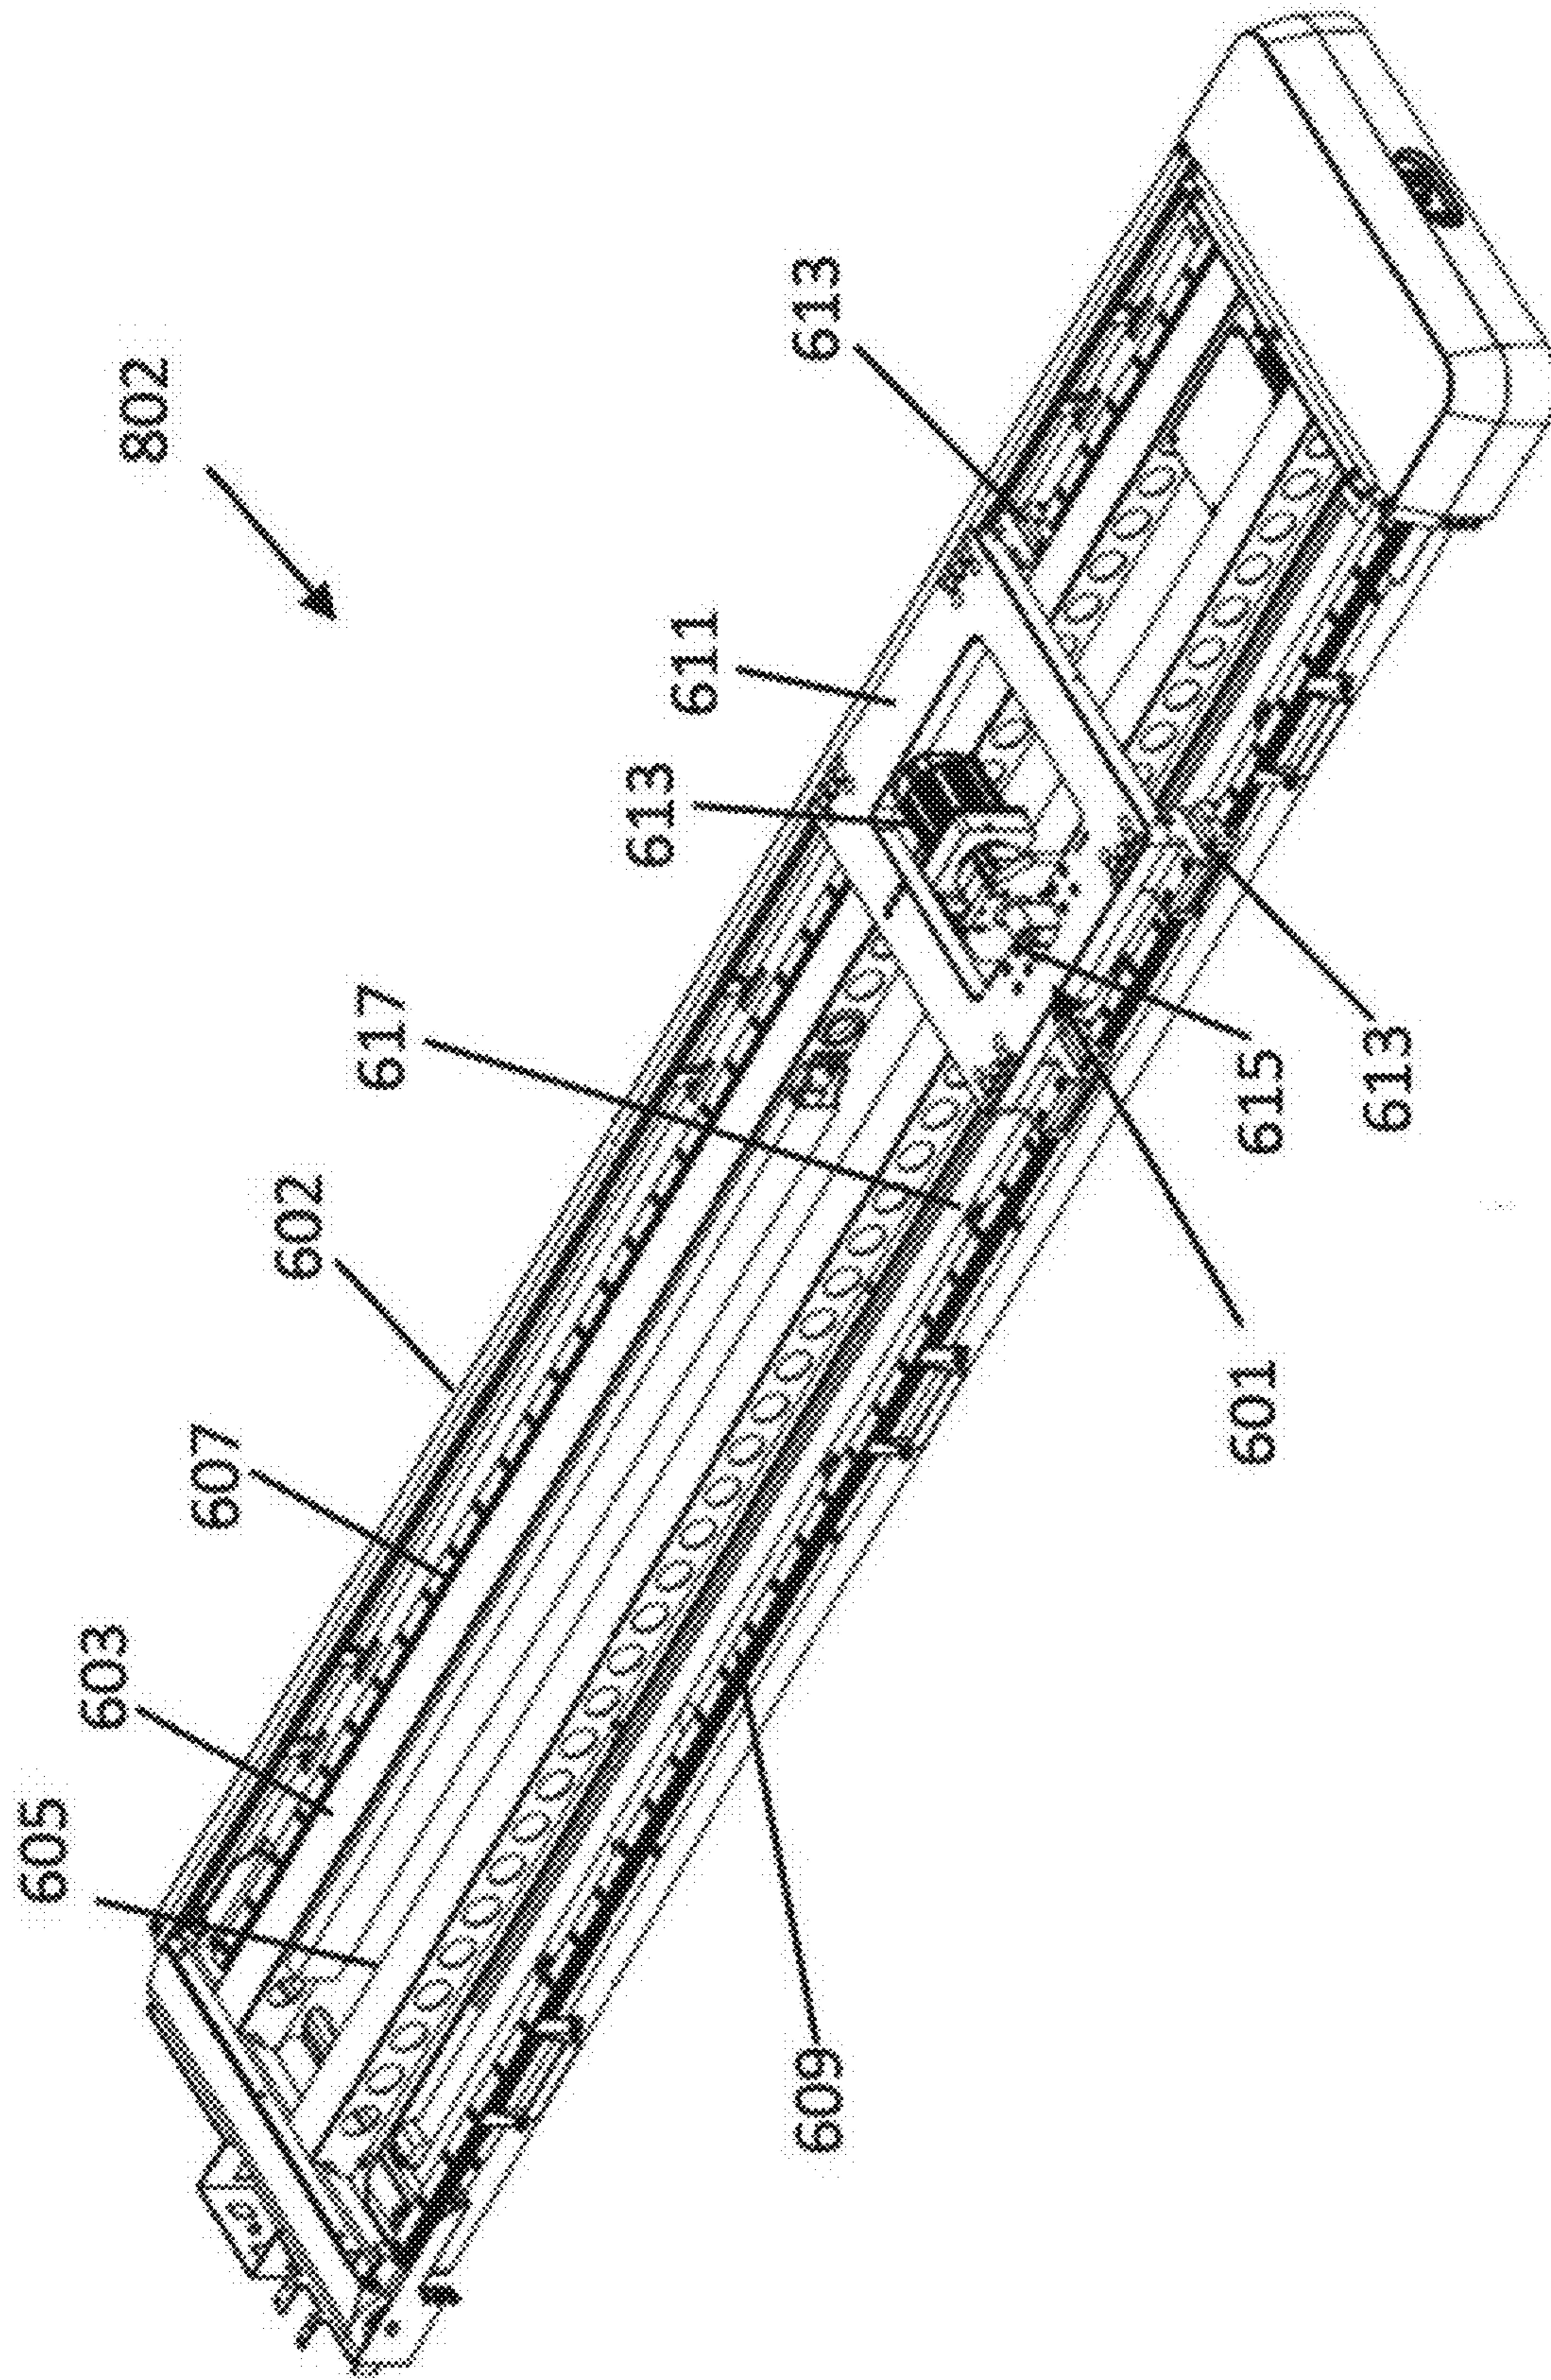


FIG. 6B

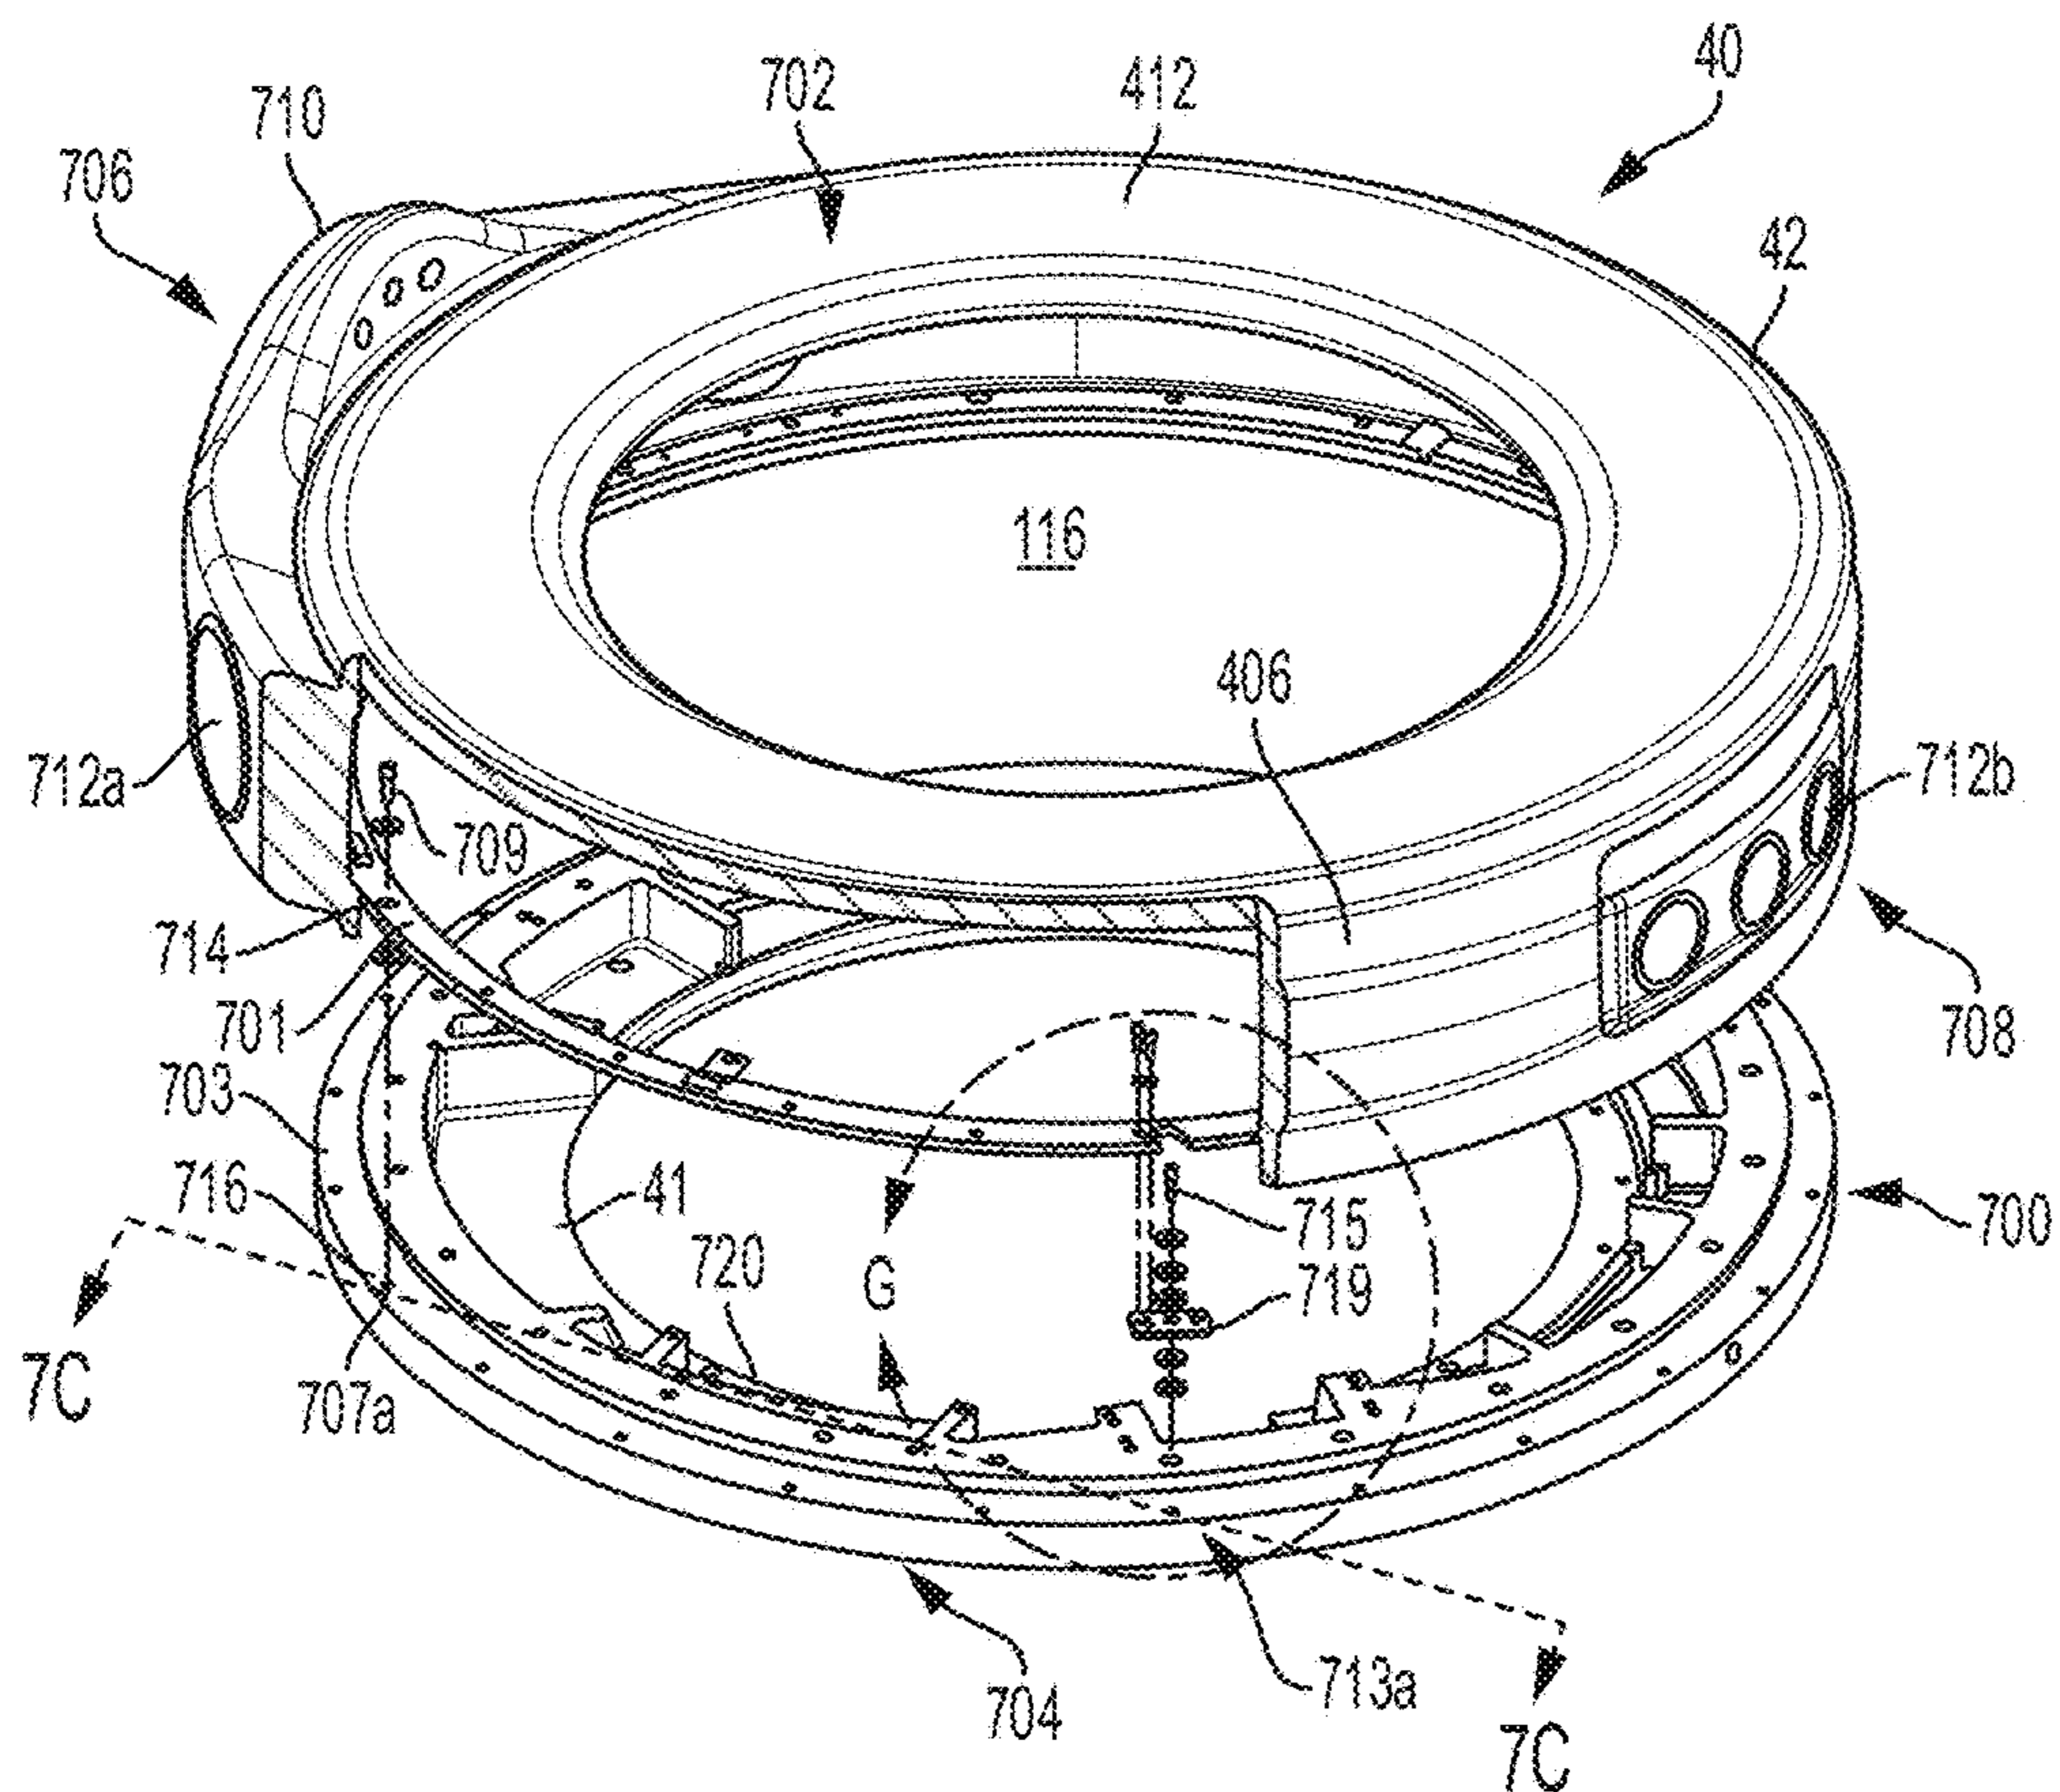


FIG. 7A



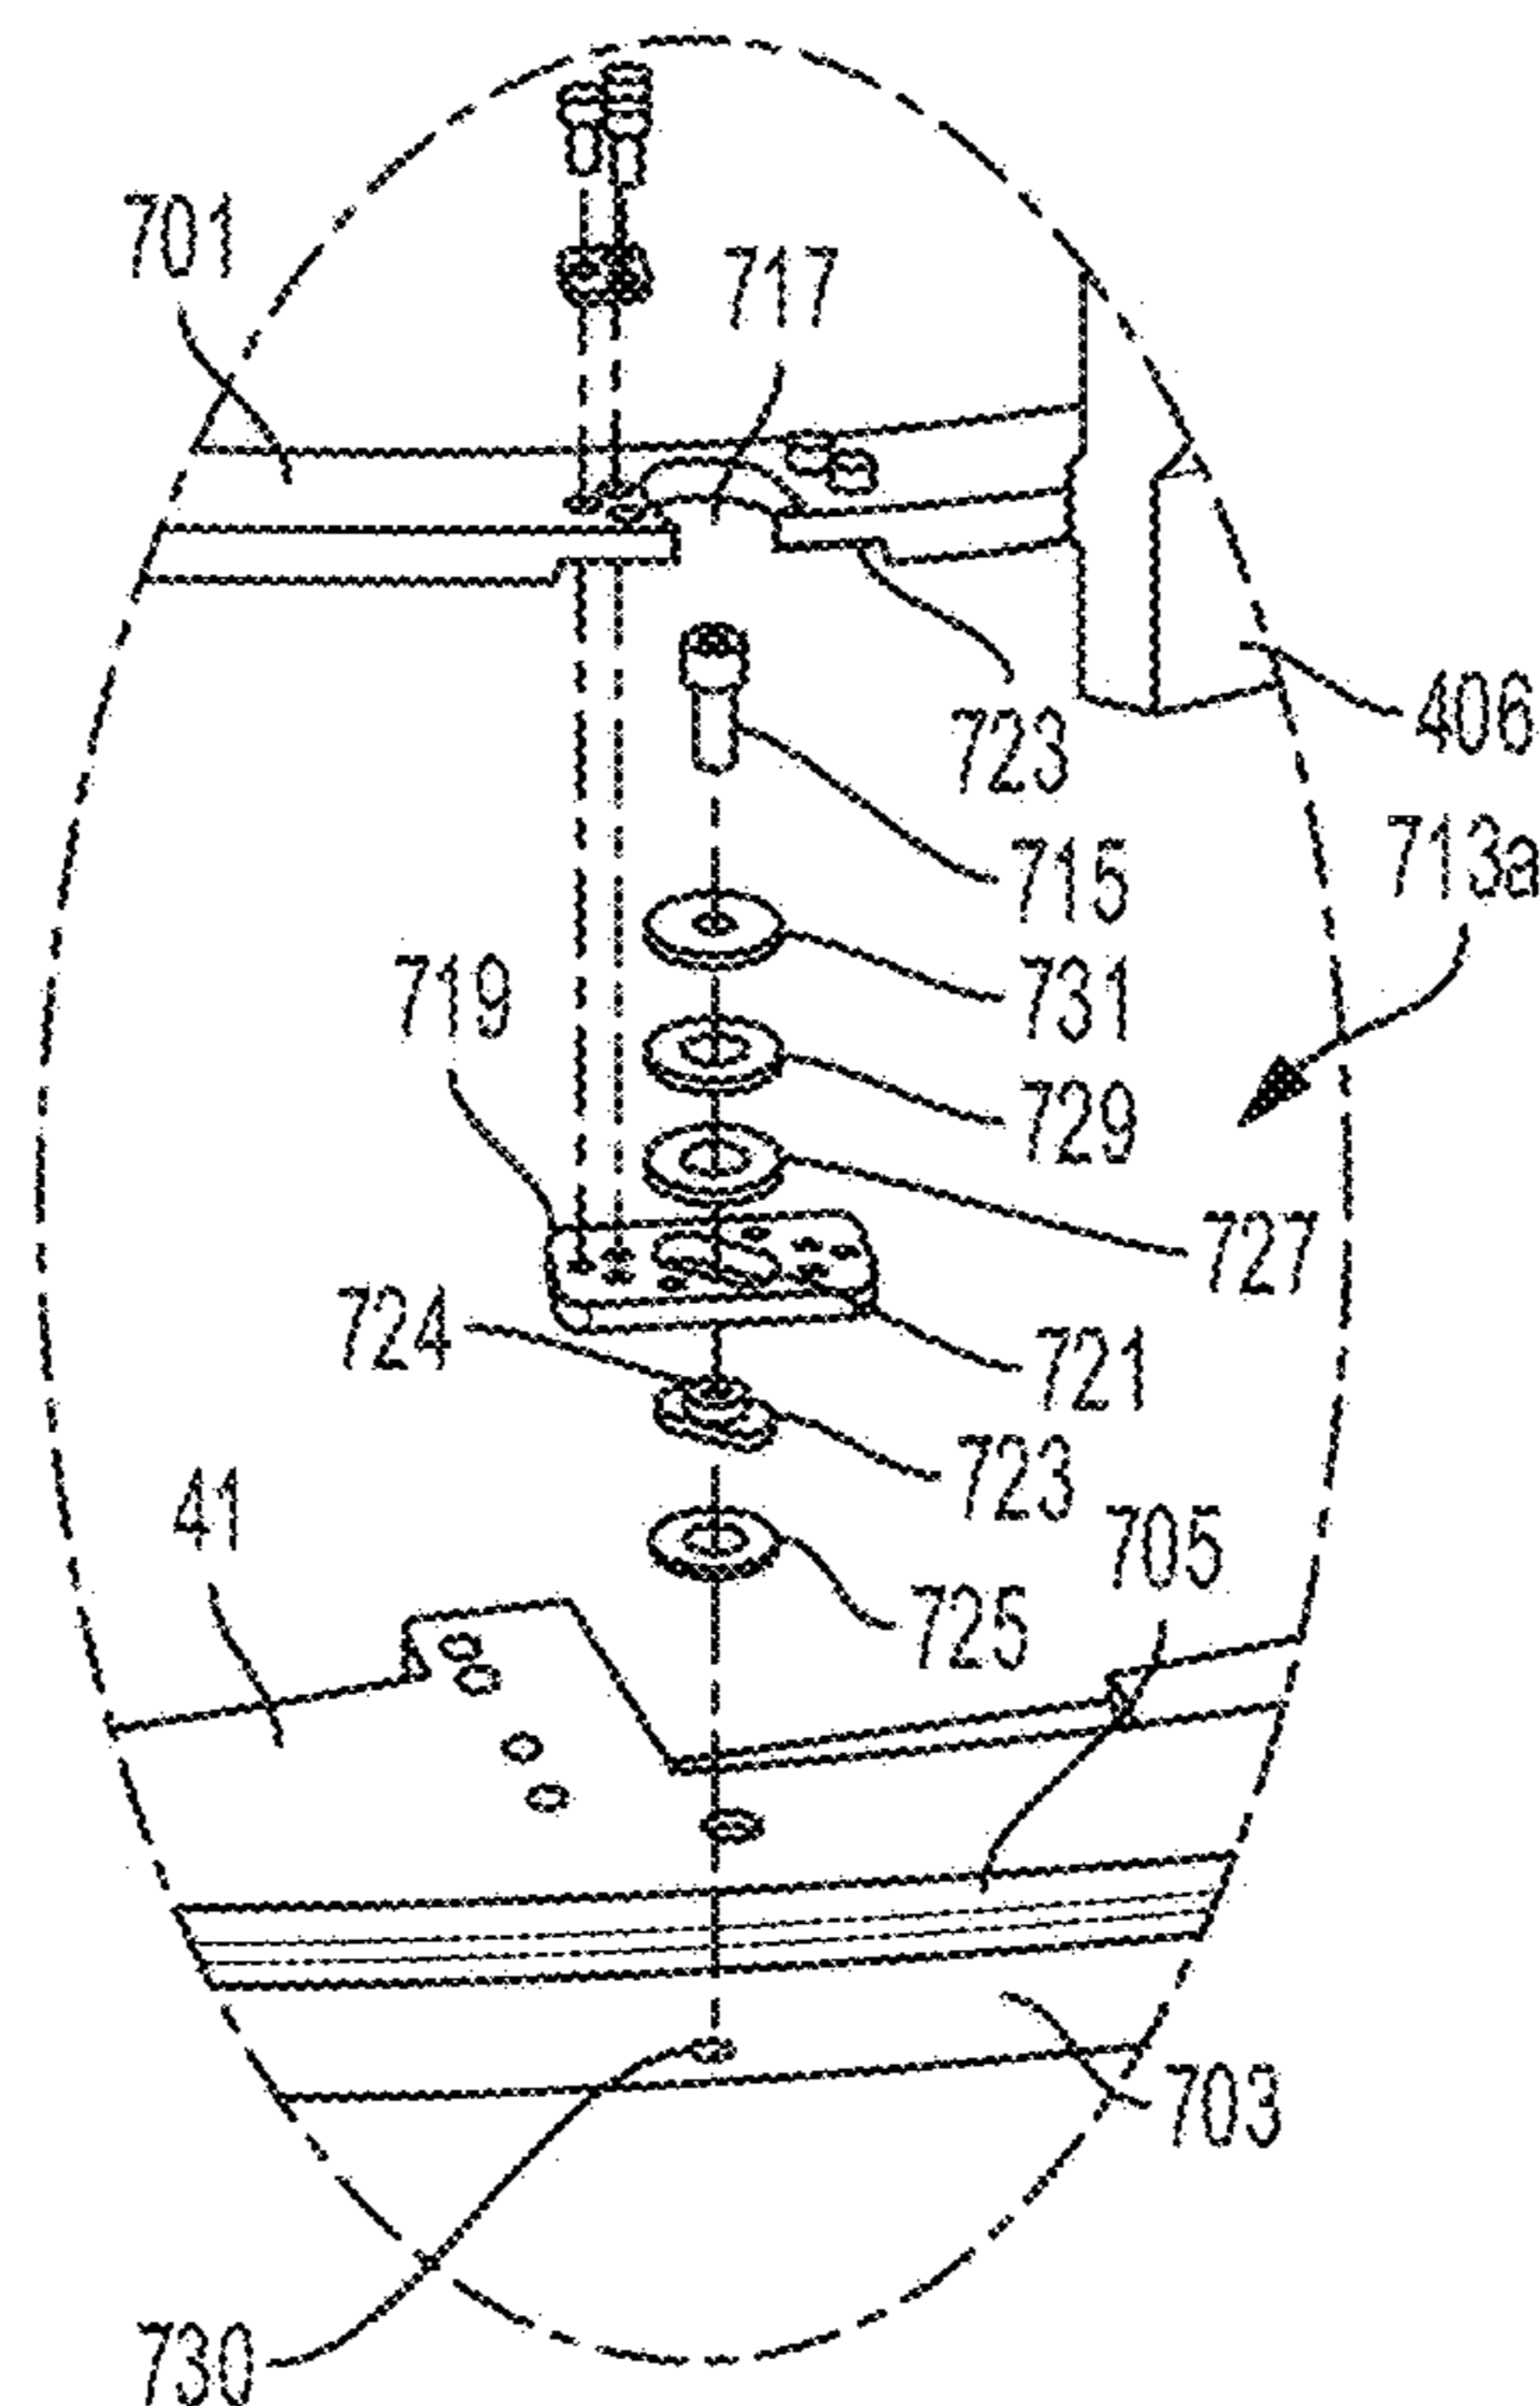


FIG. 7B

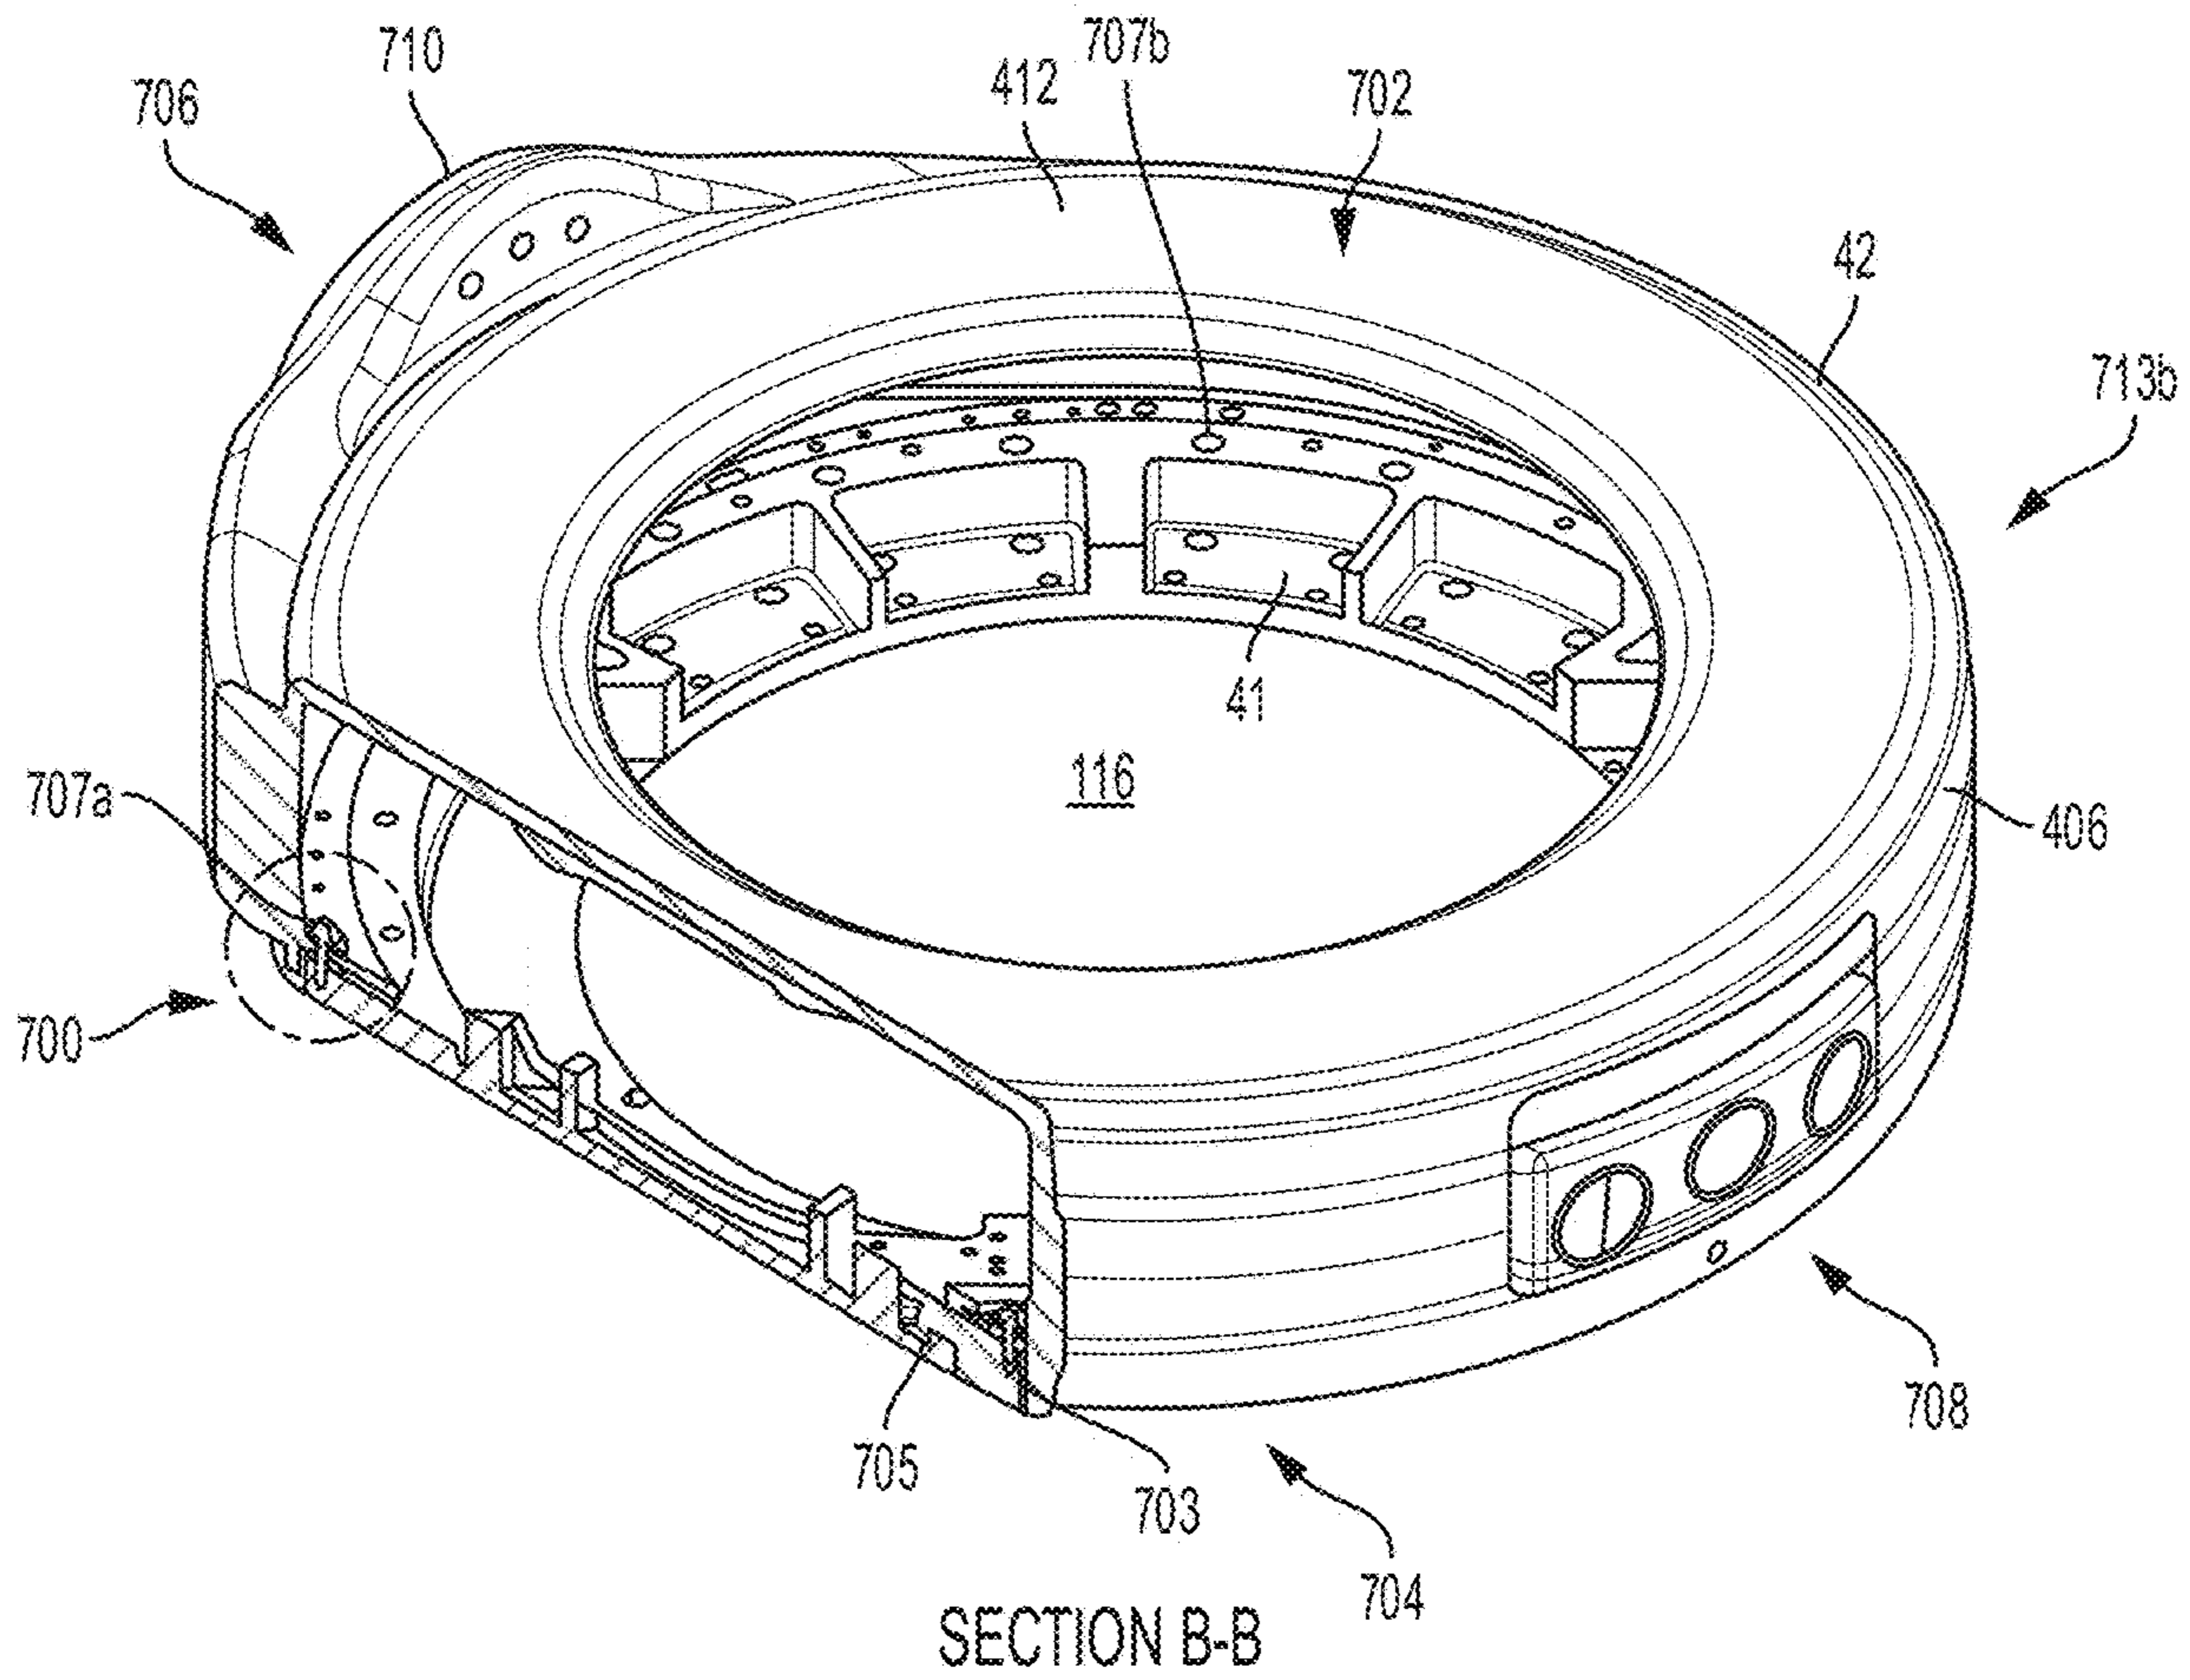


SECTION B-B

FIG. 7C

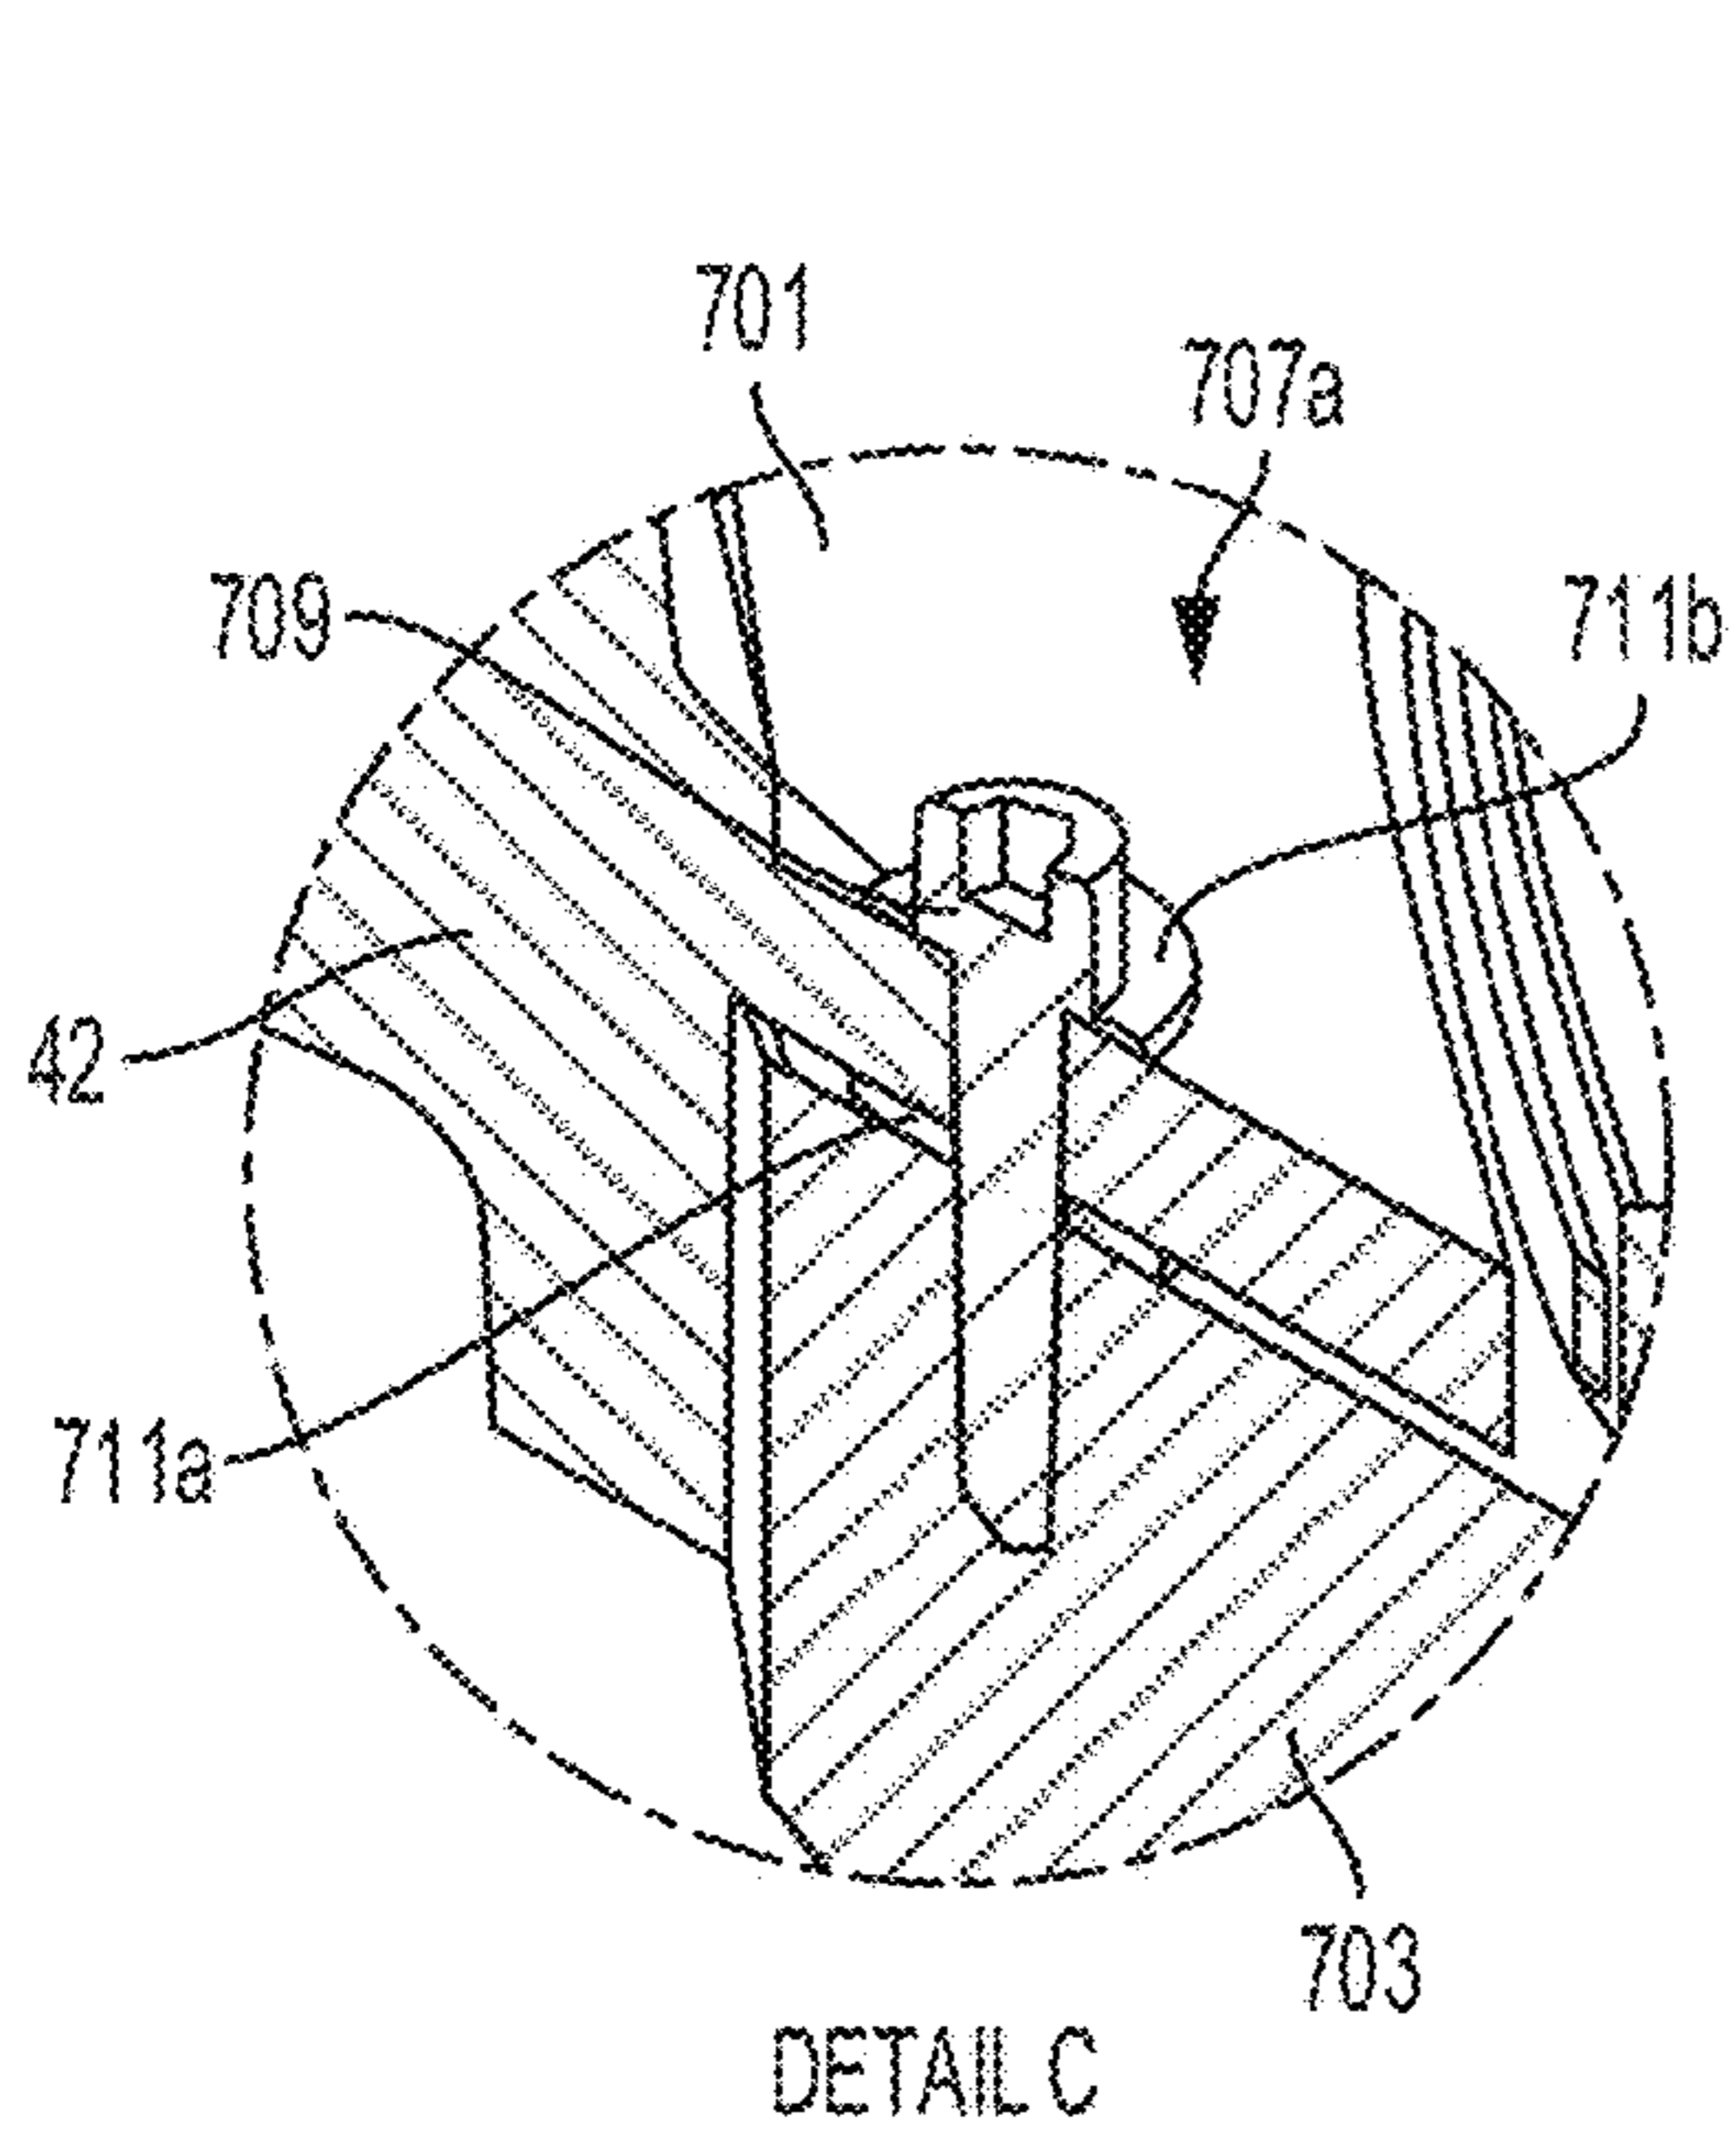

DETAIL C

FIG. 7D

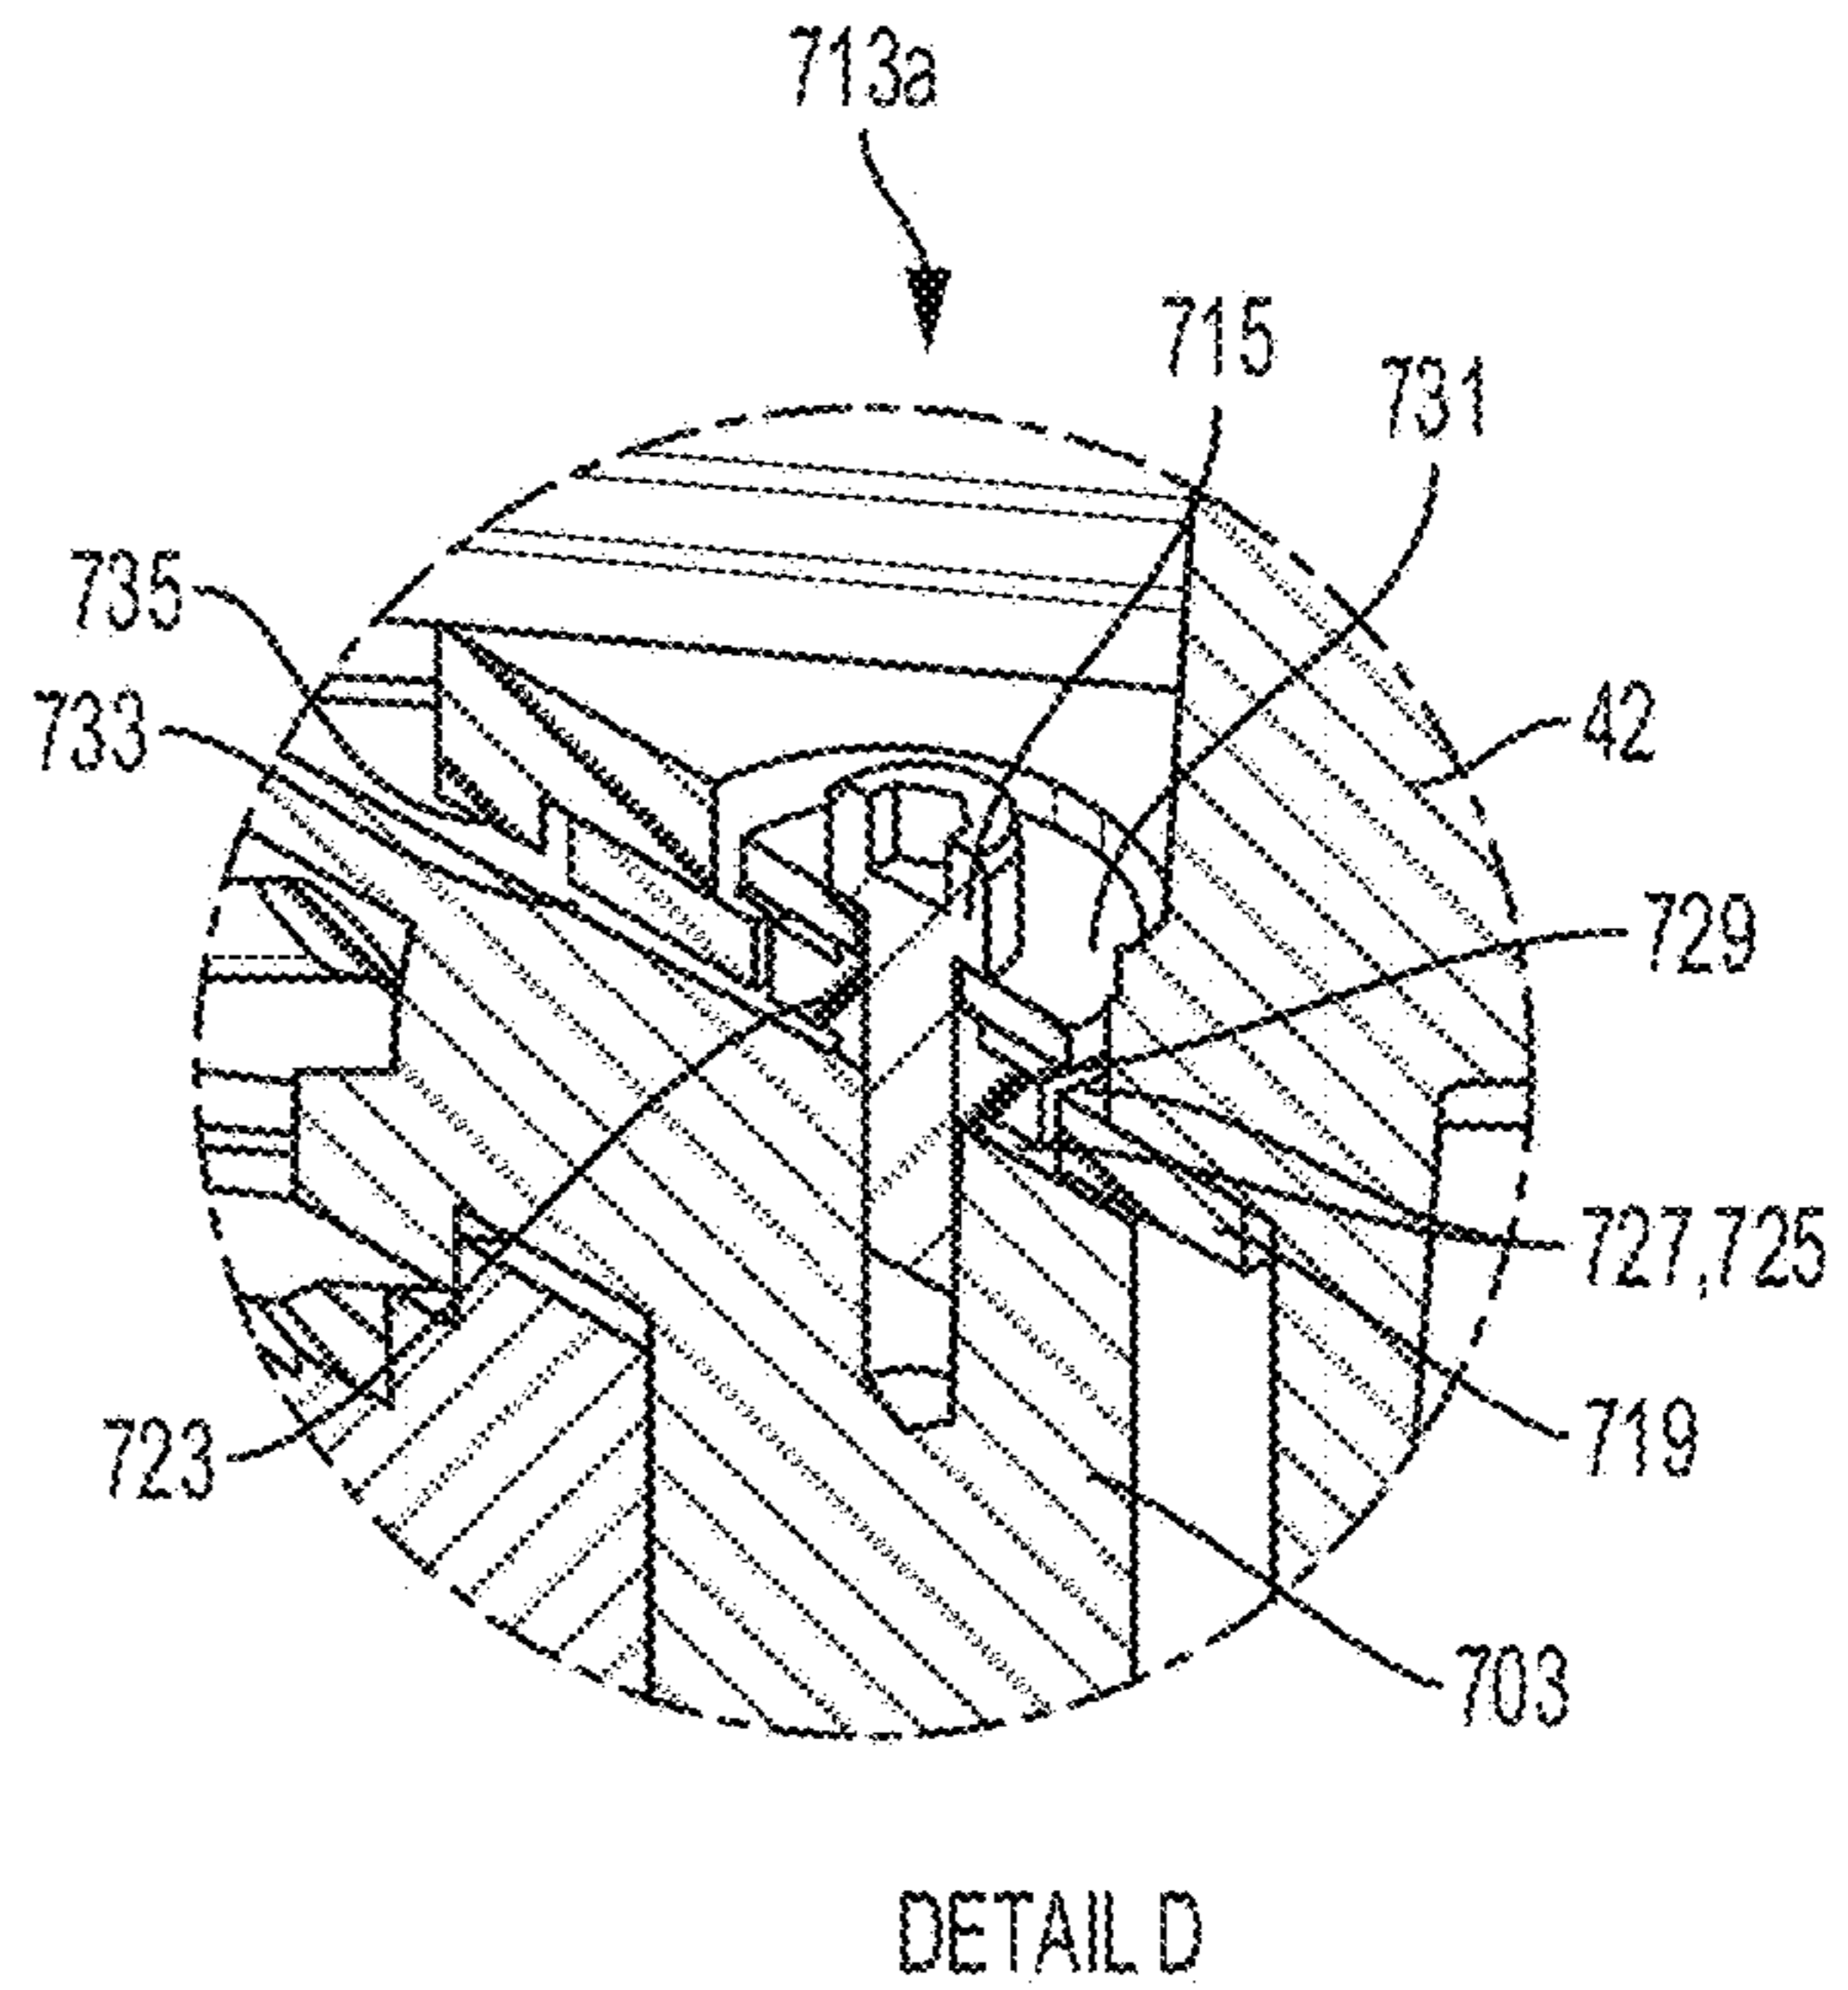

DETAIL D

FIG. 7E

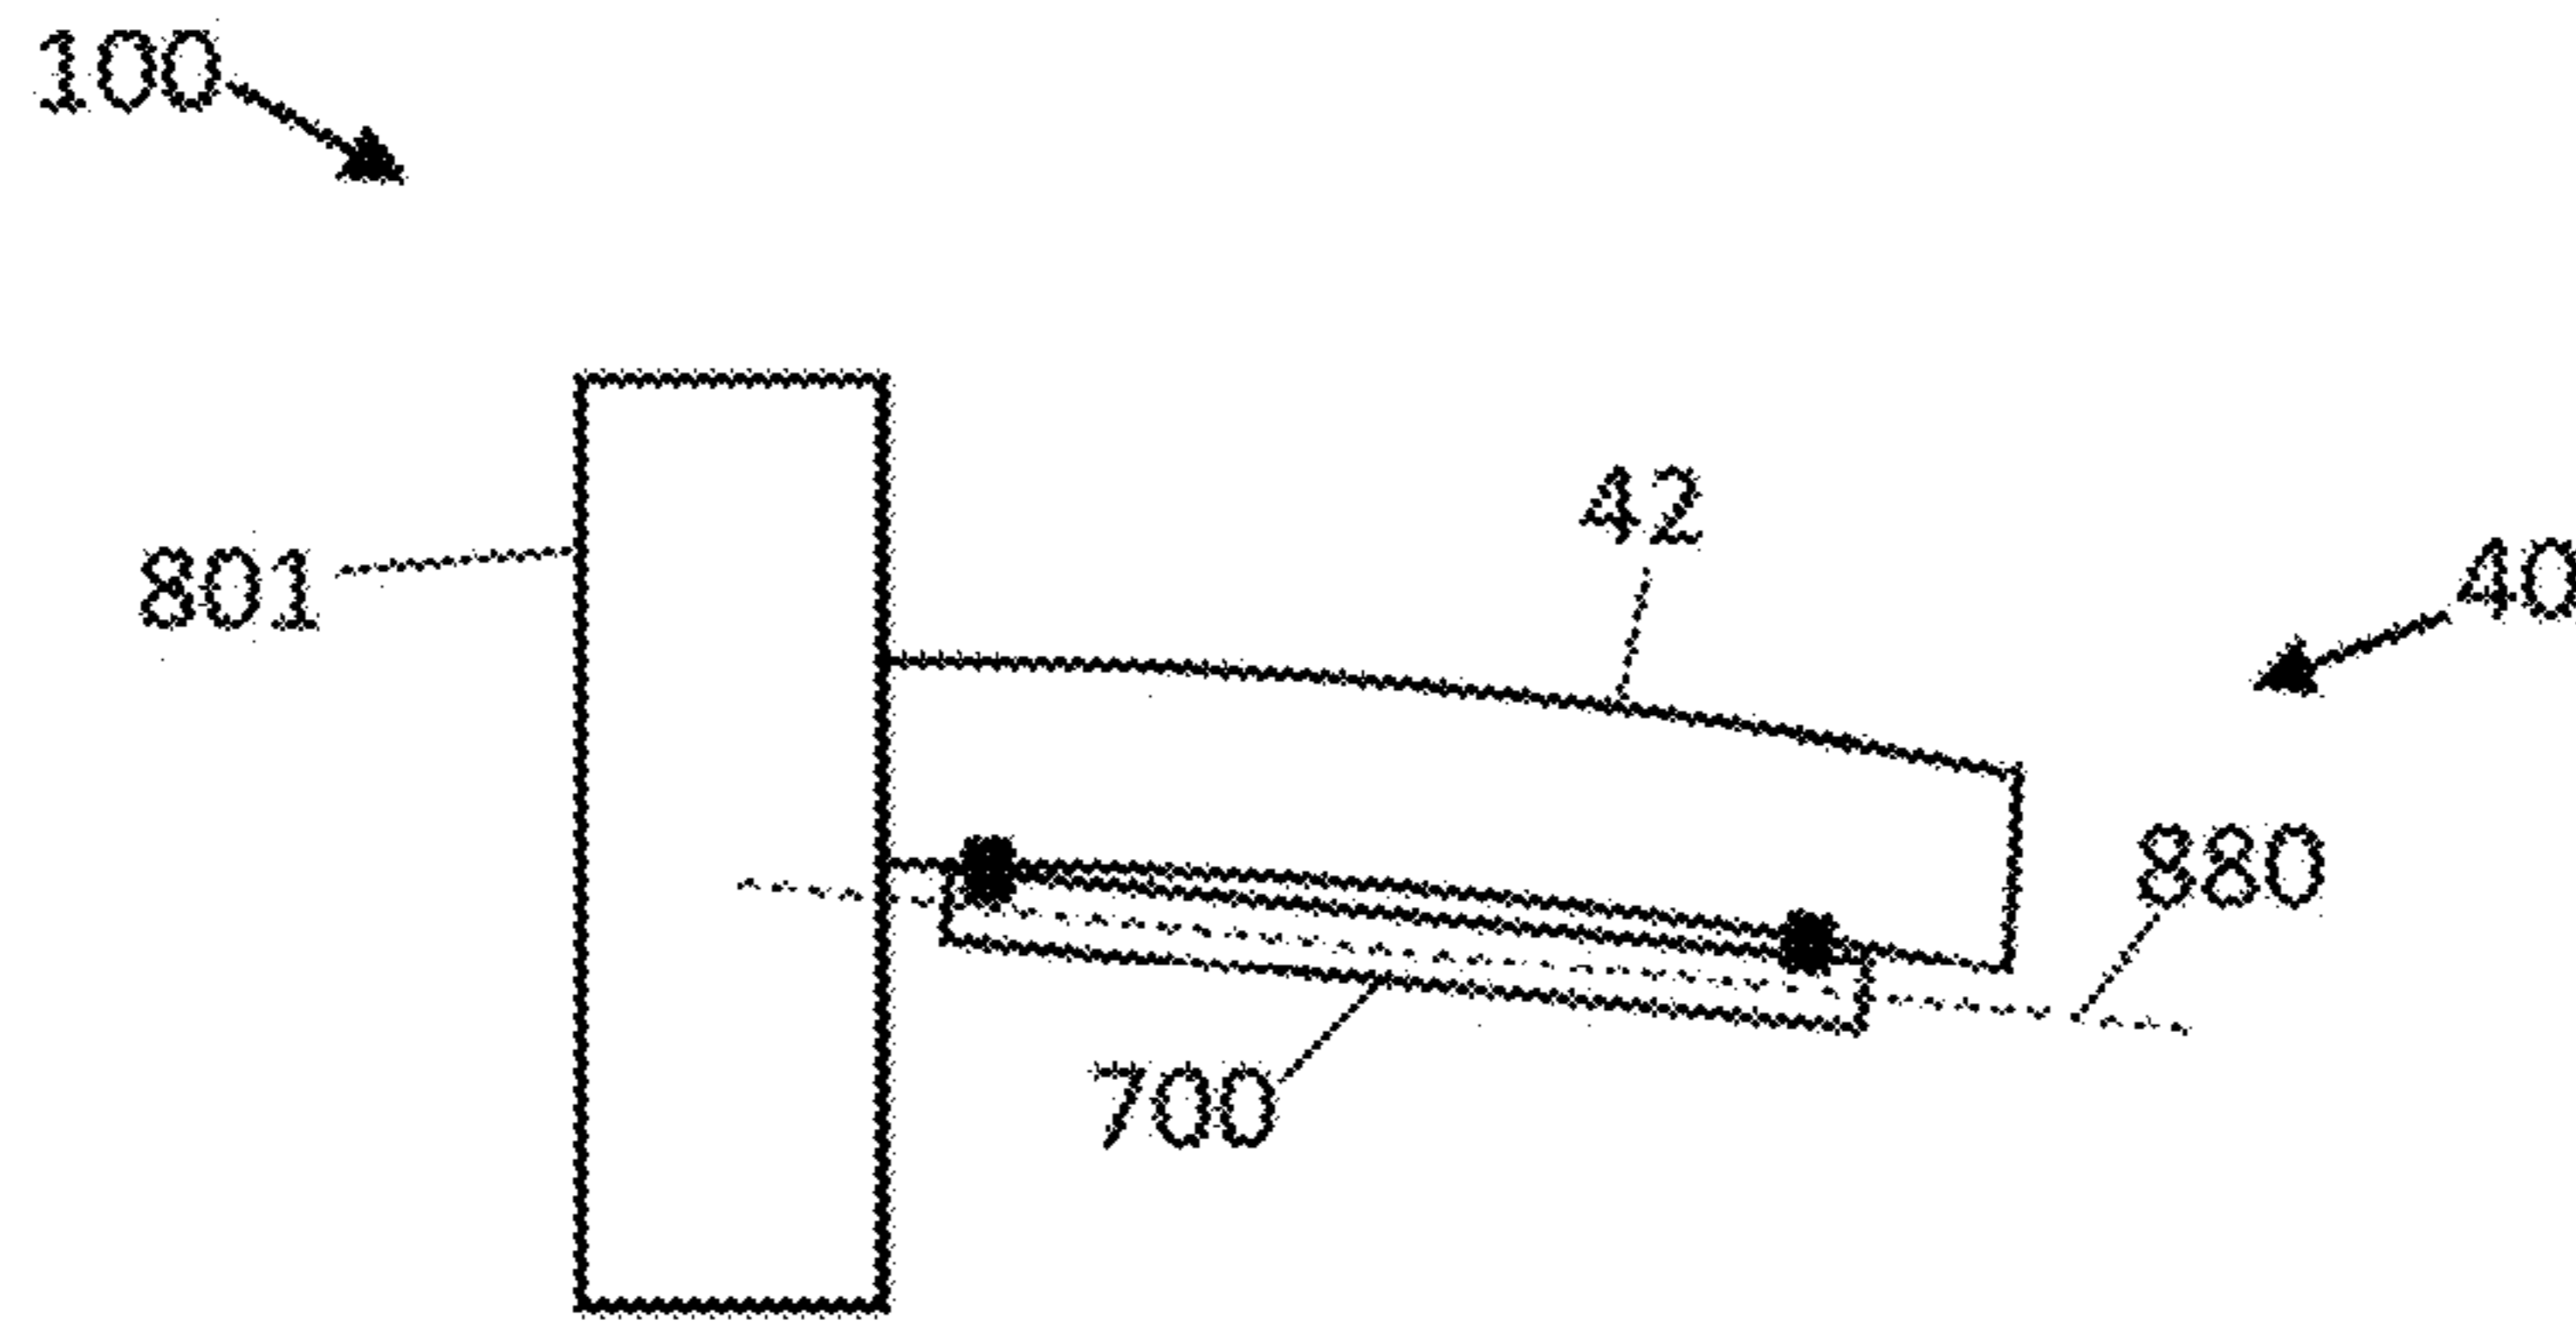


FIG. 8

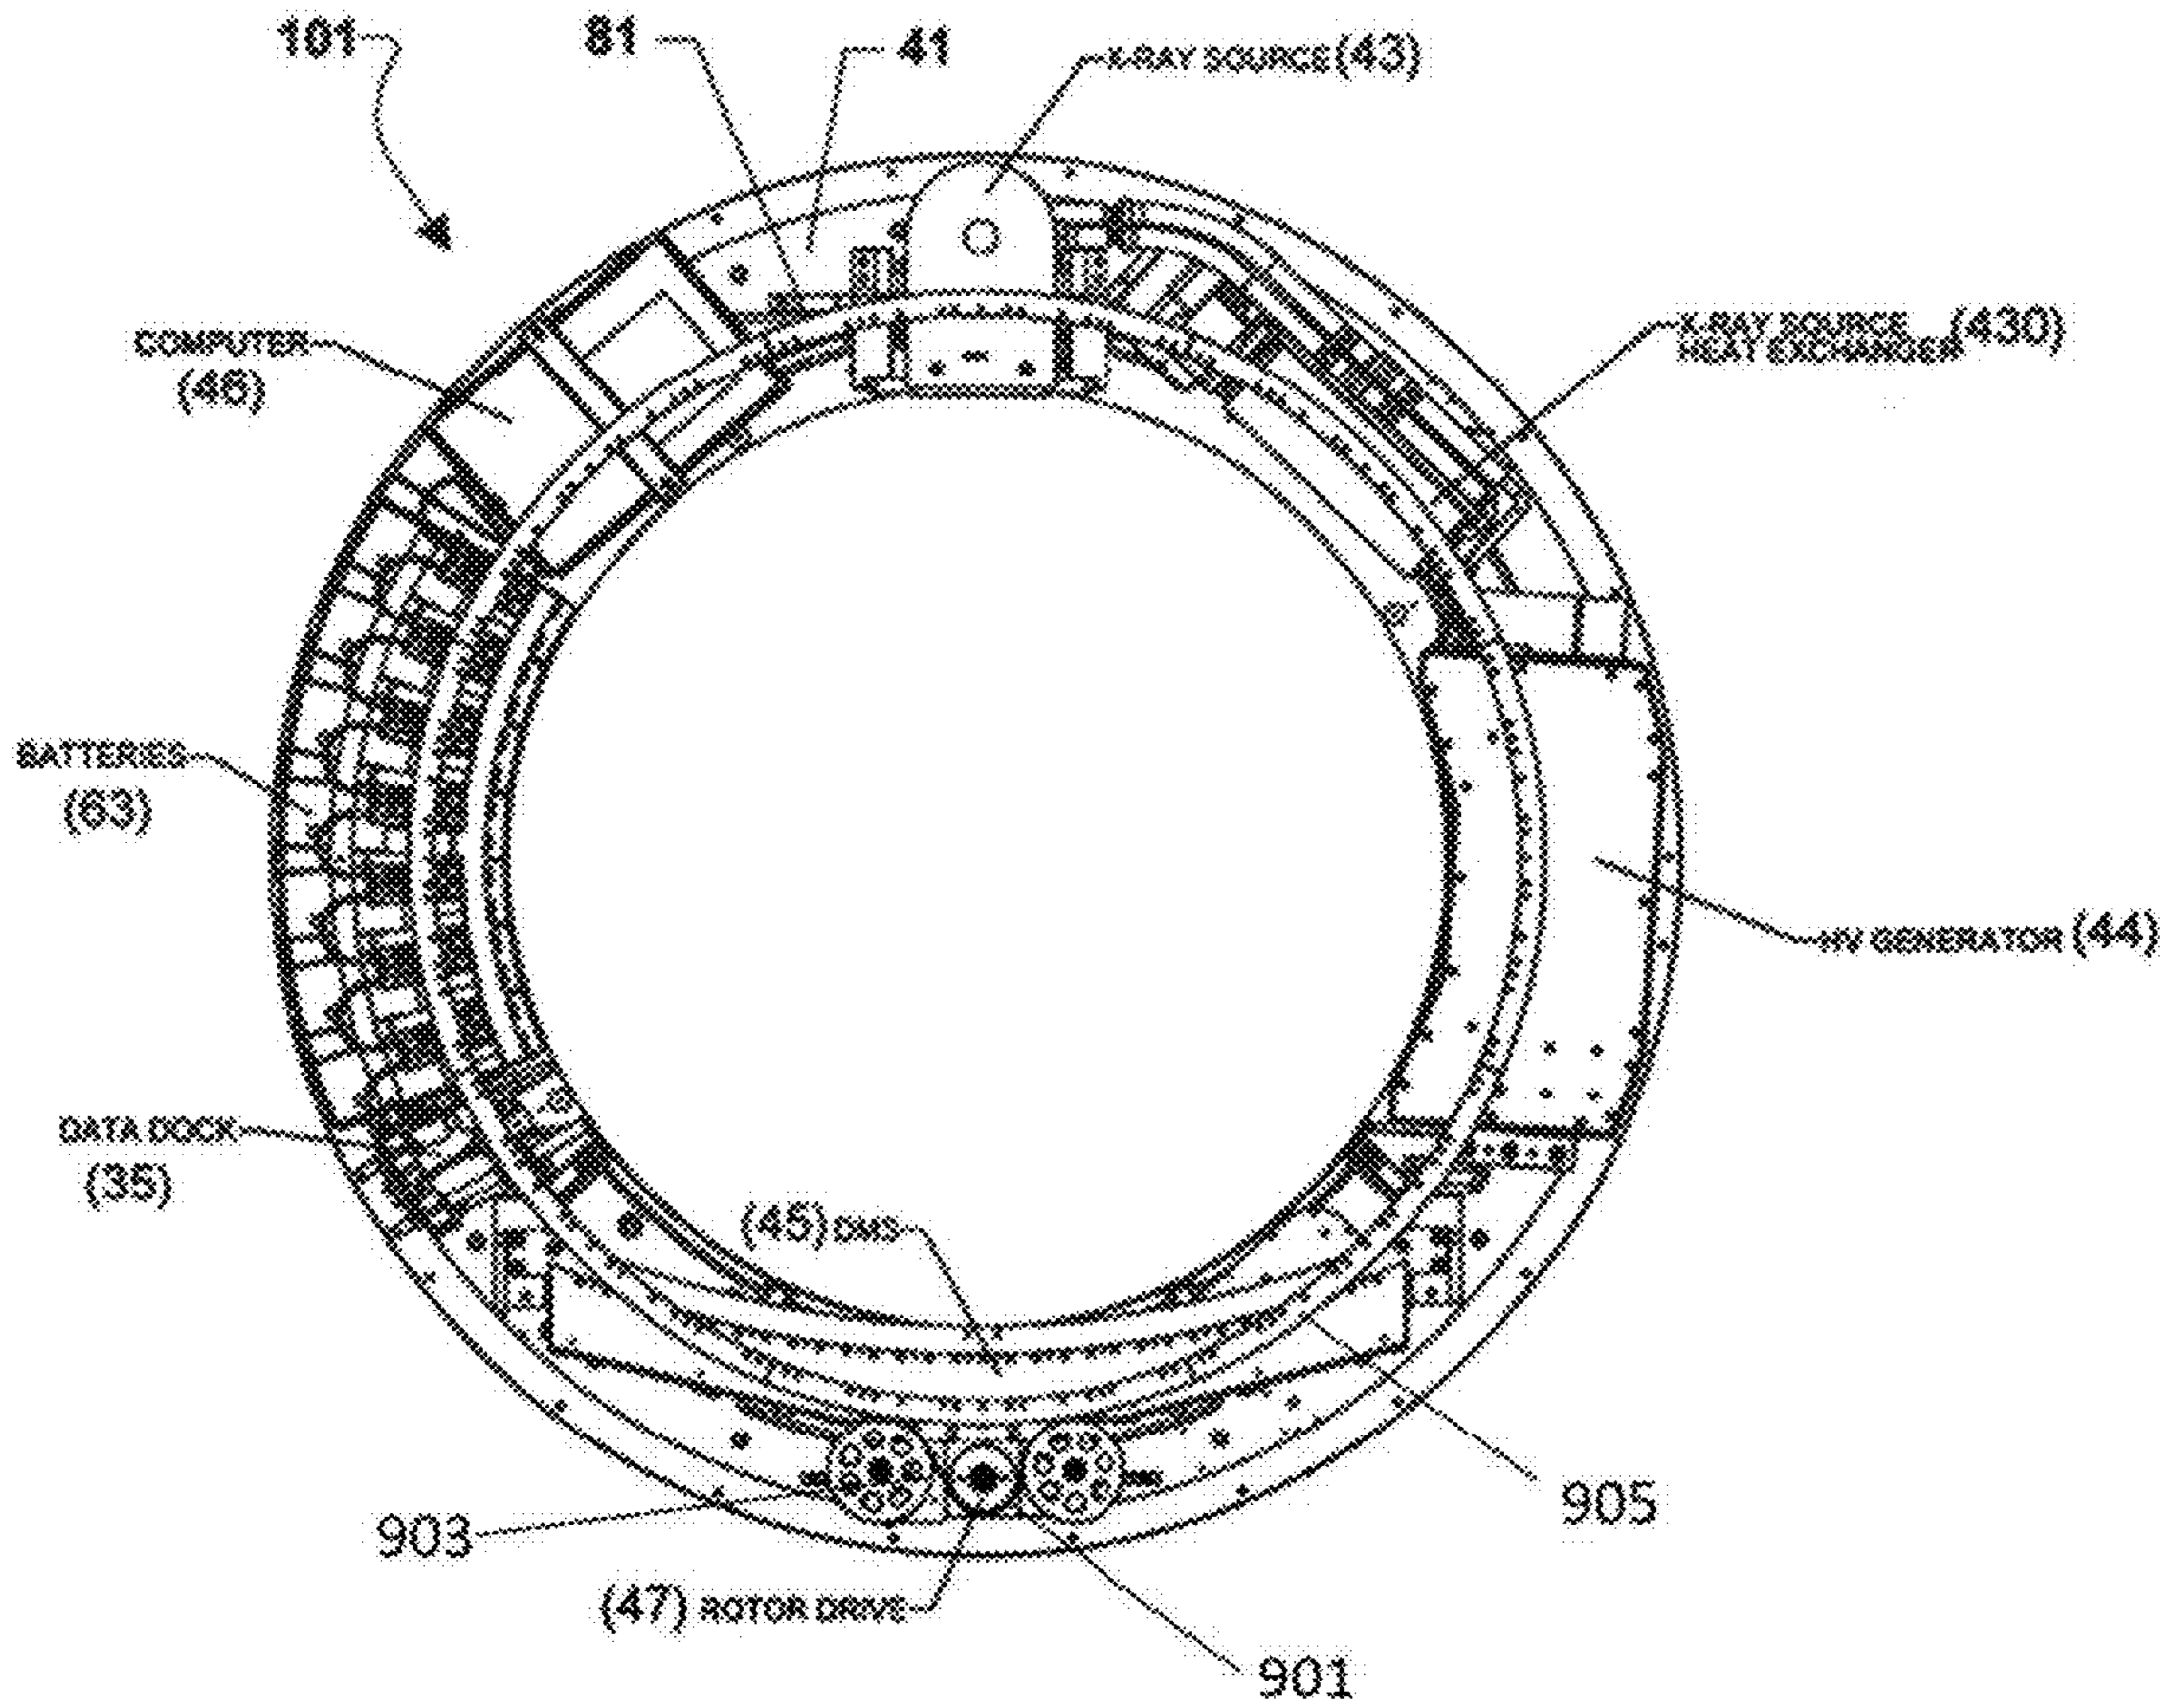


FIG. 9

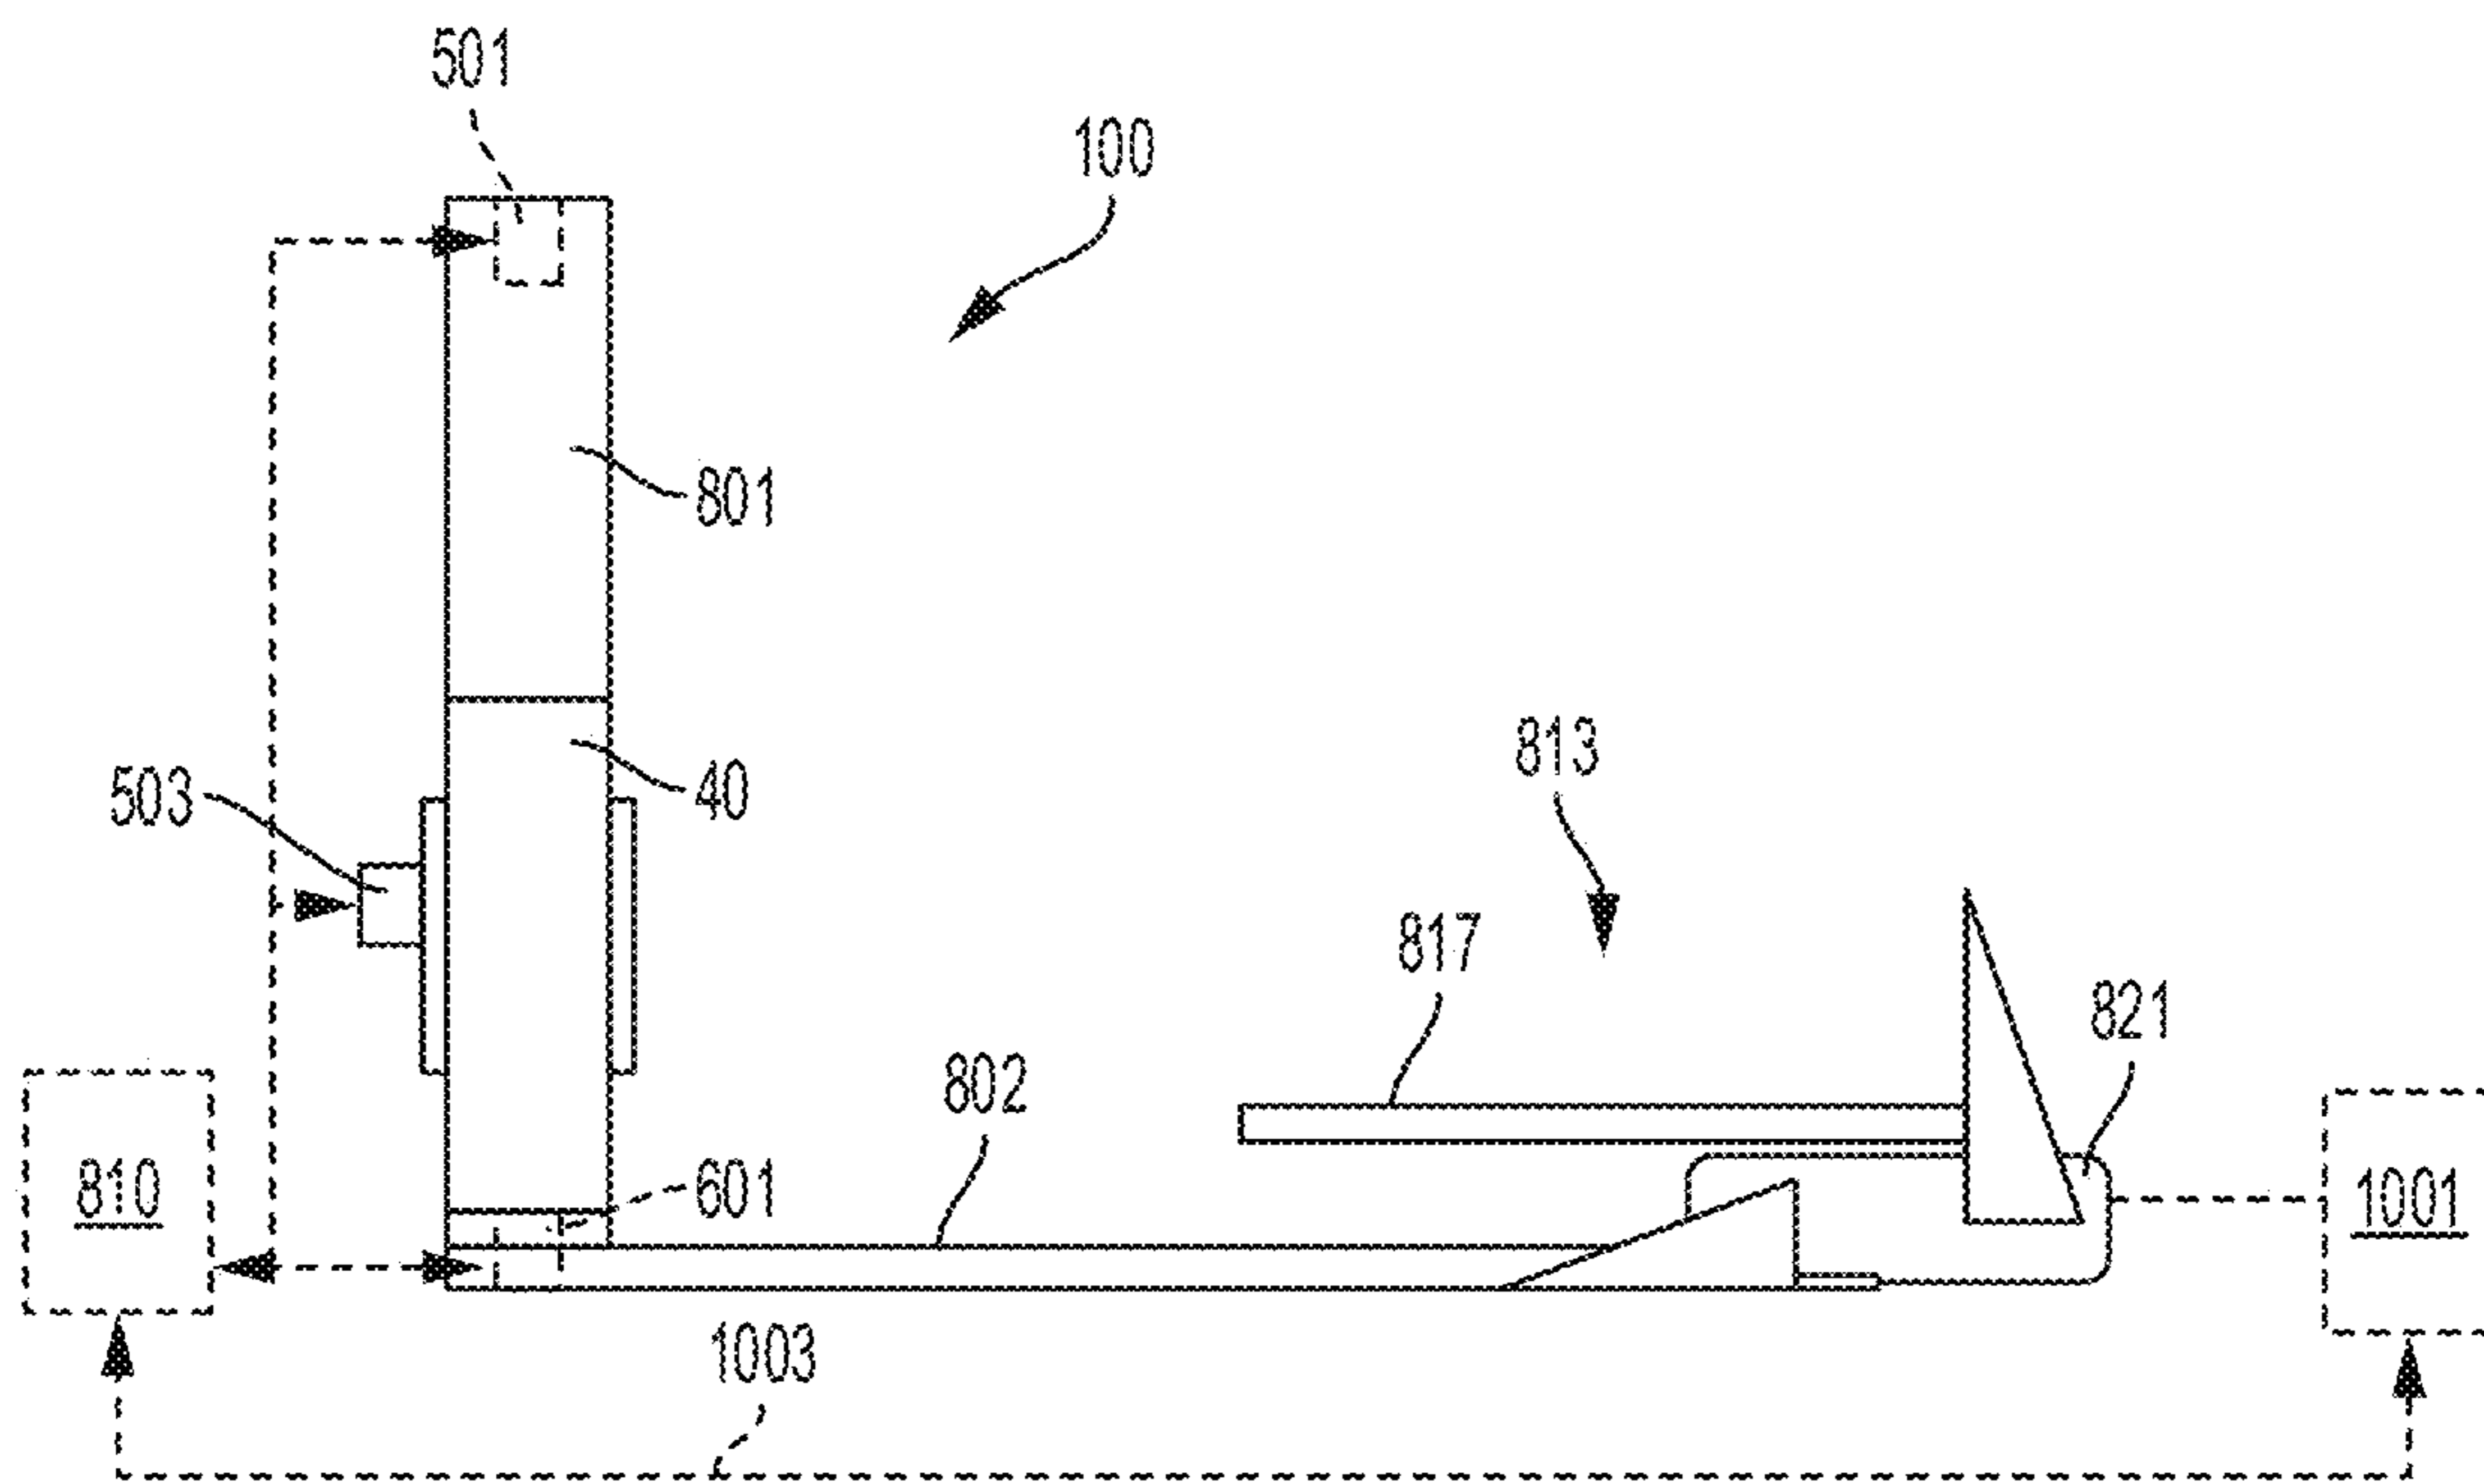


FIG. 10A

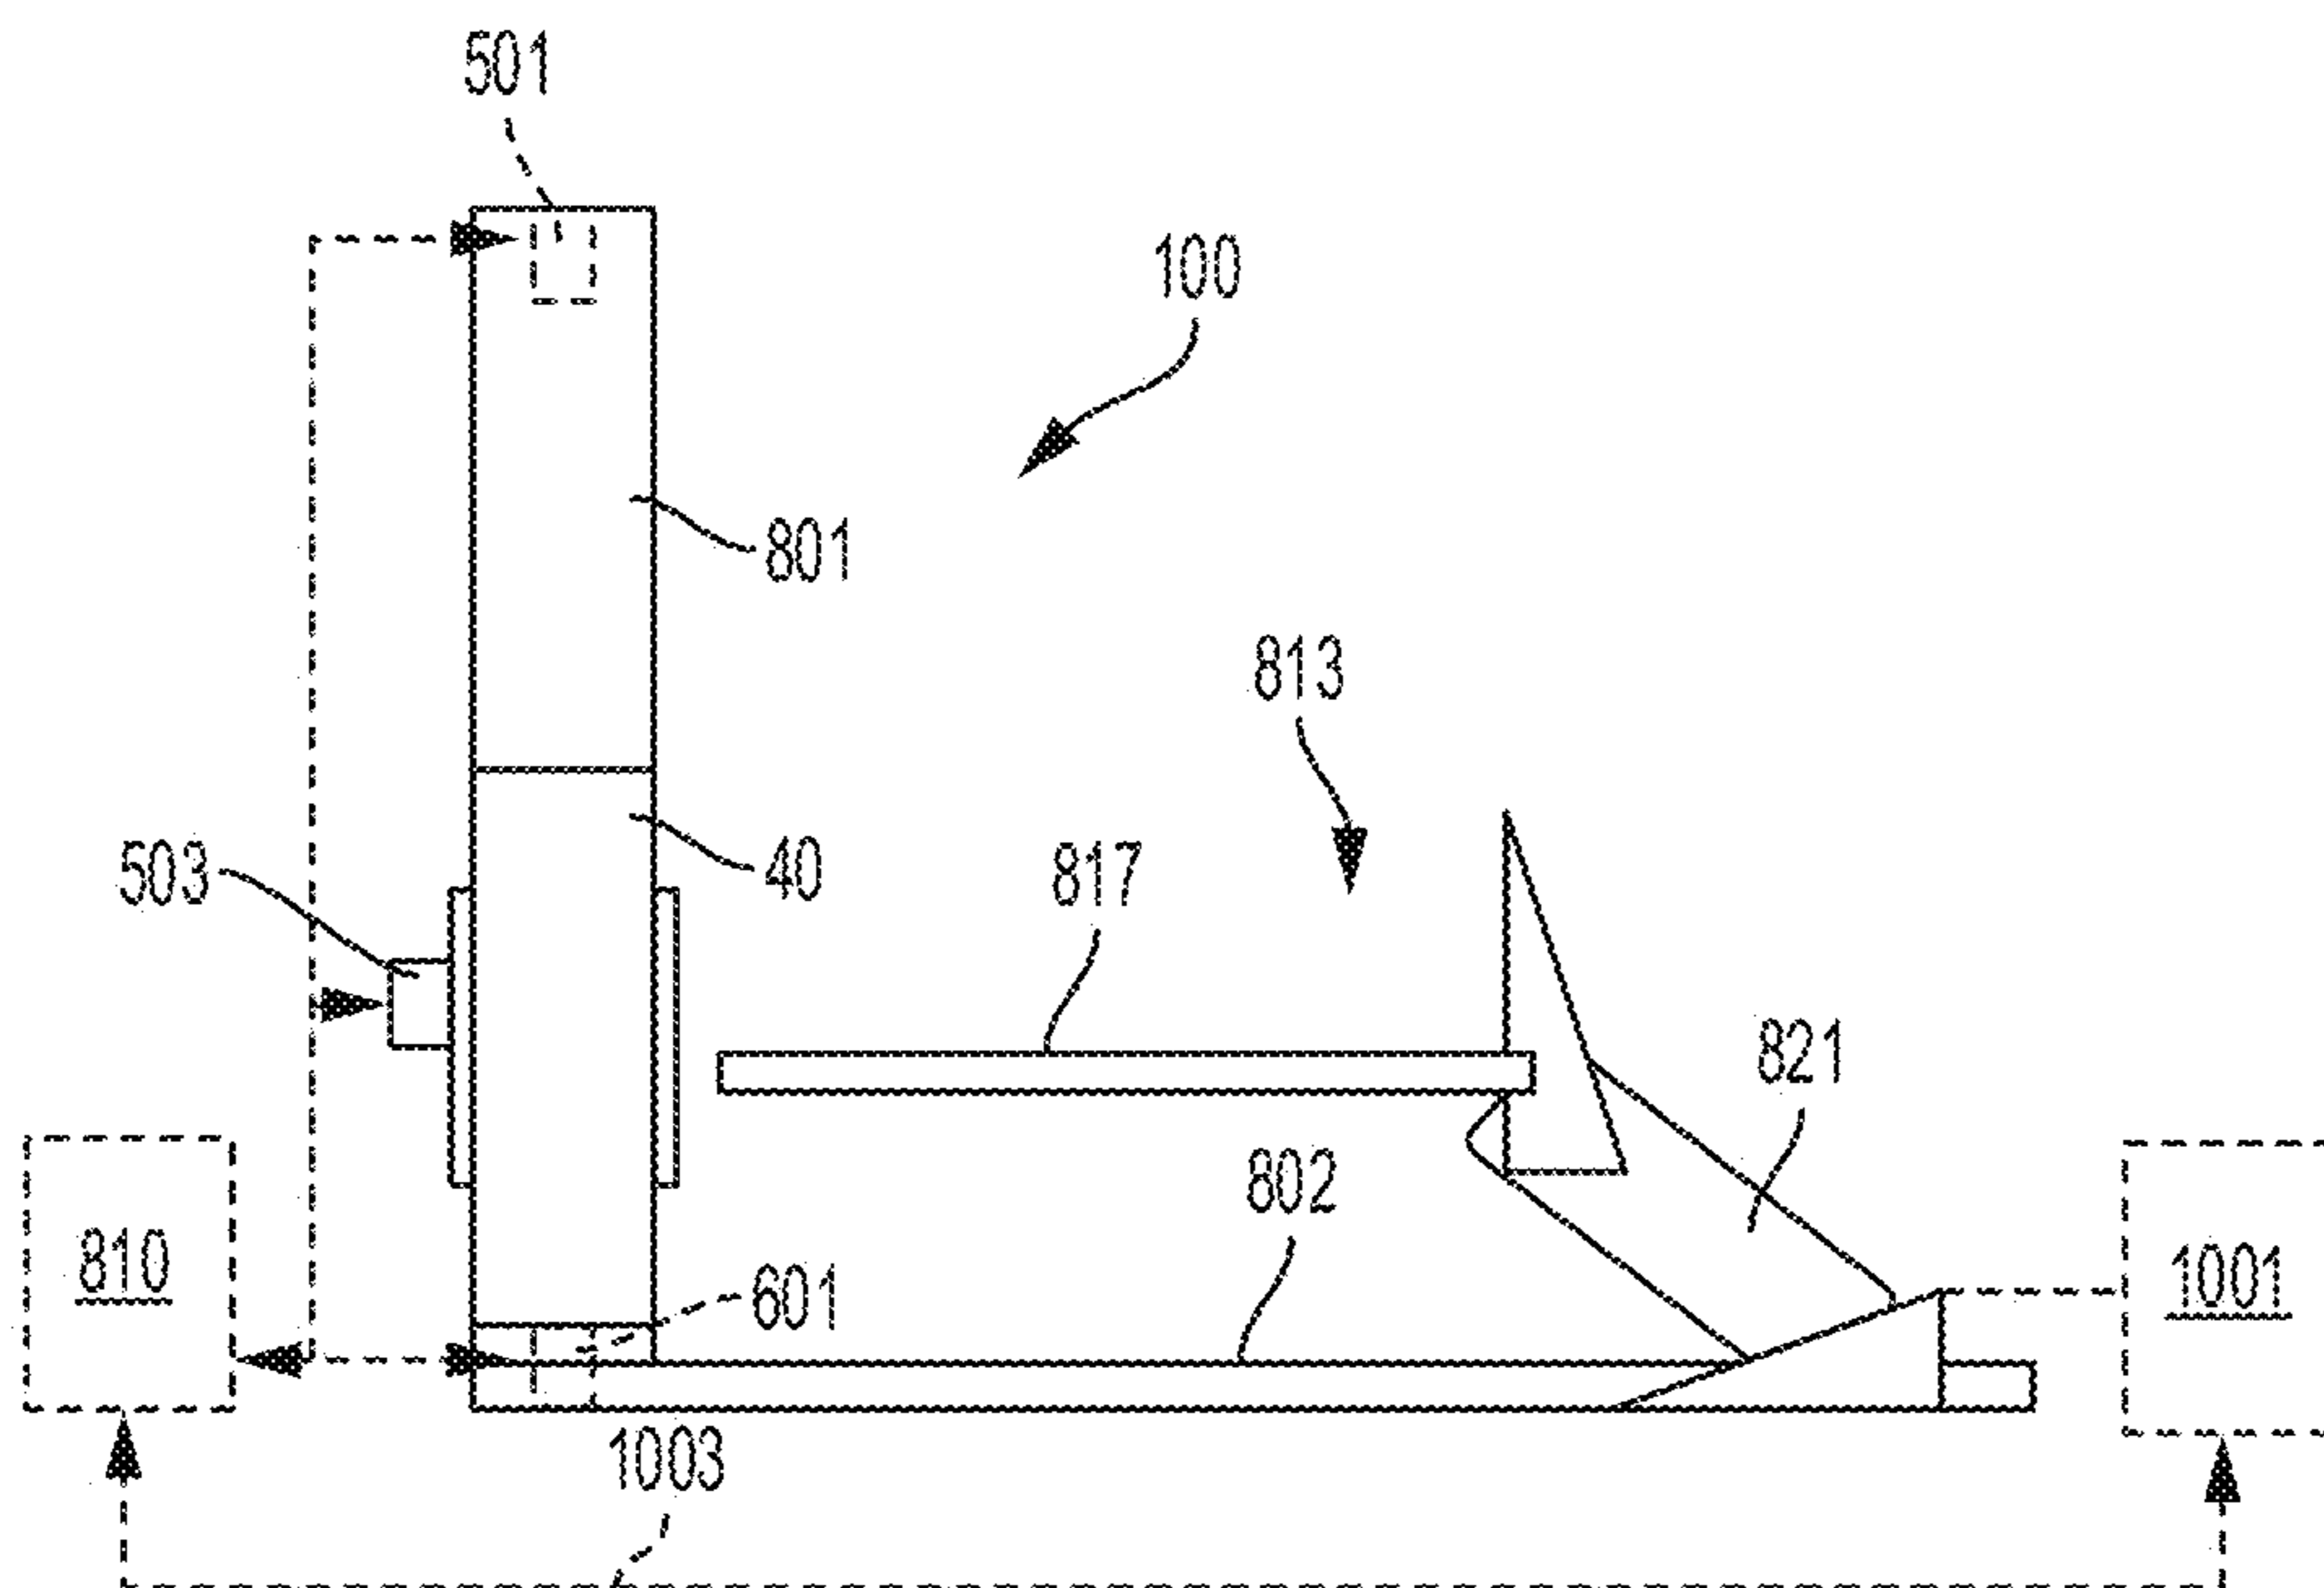


FIG. 10B

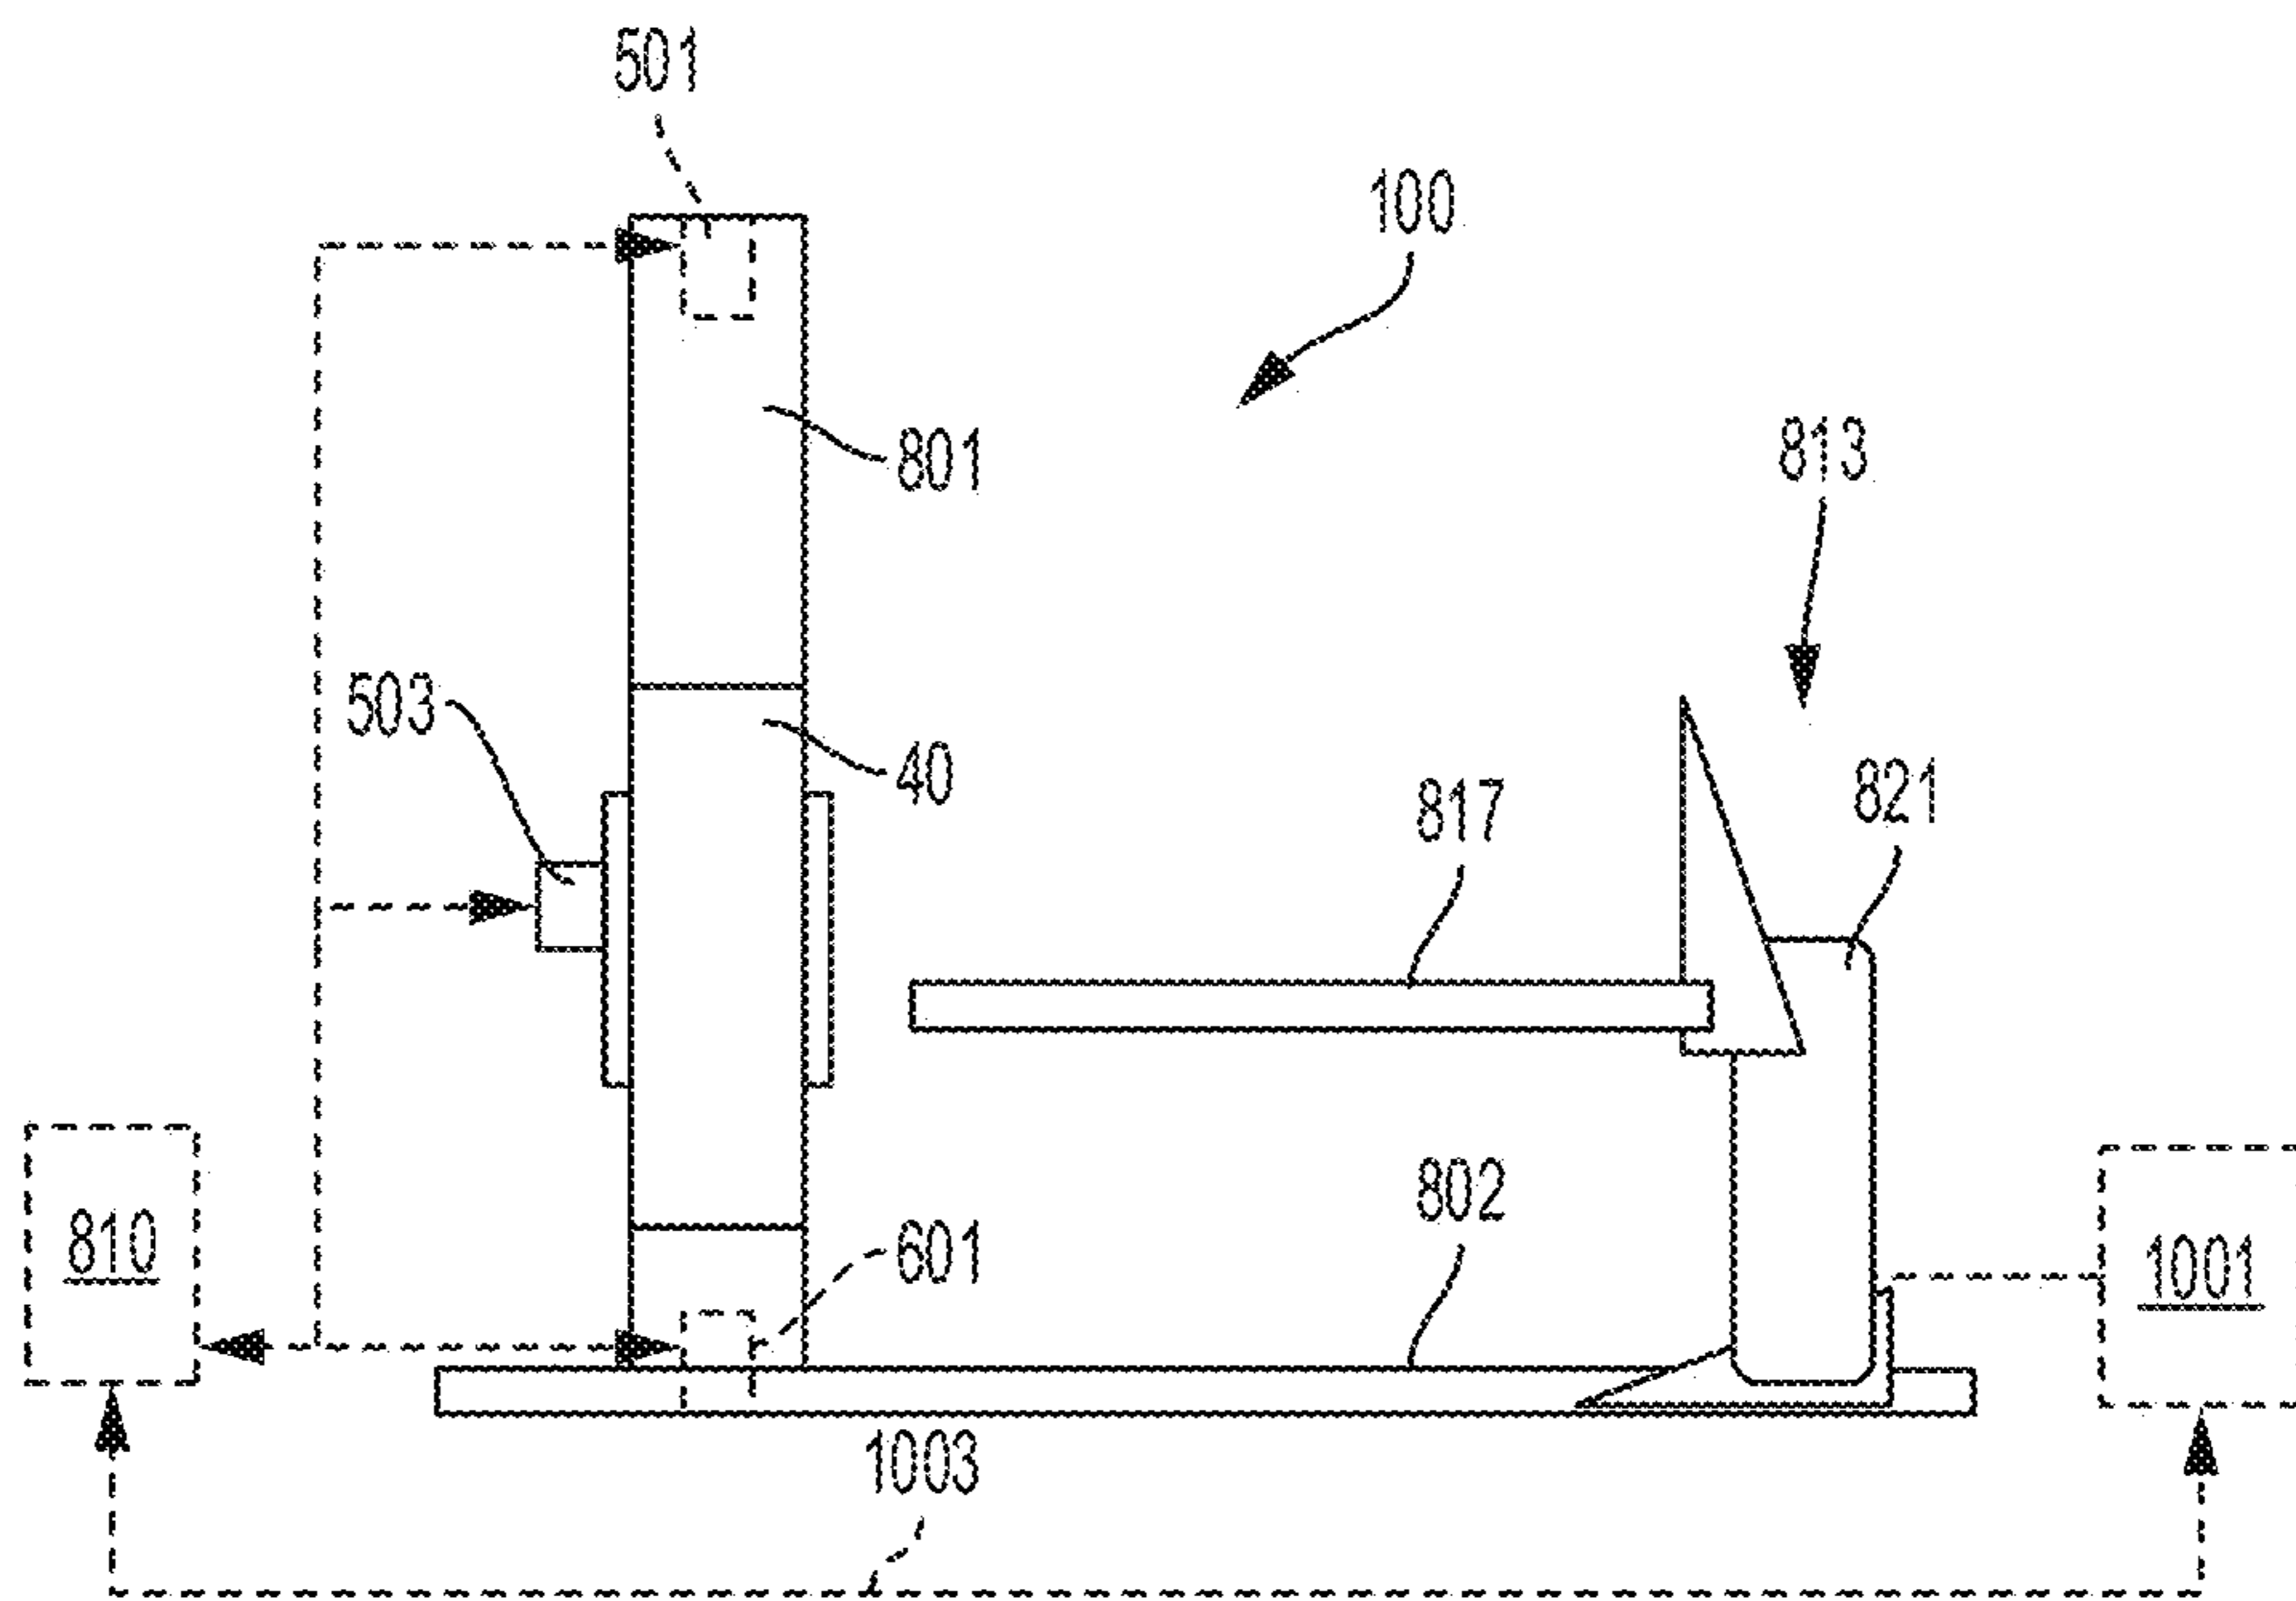


FIG. 10C

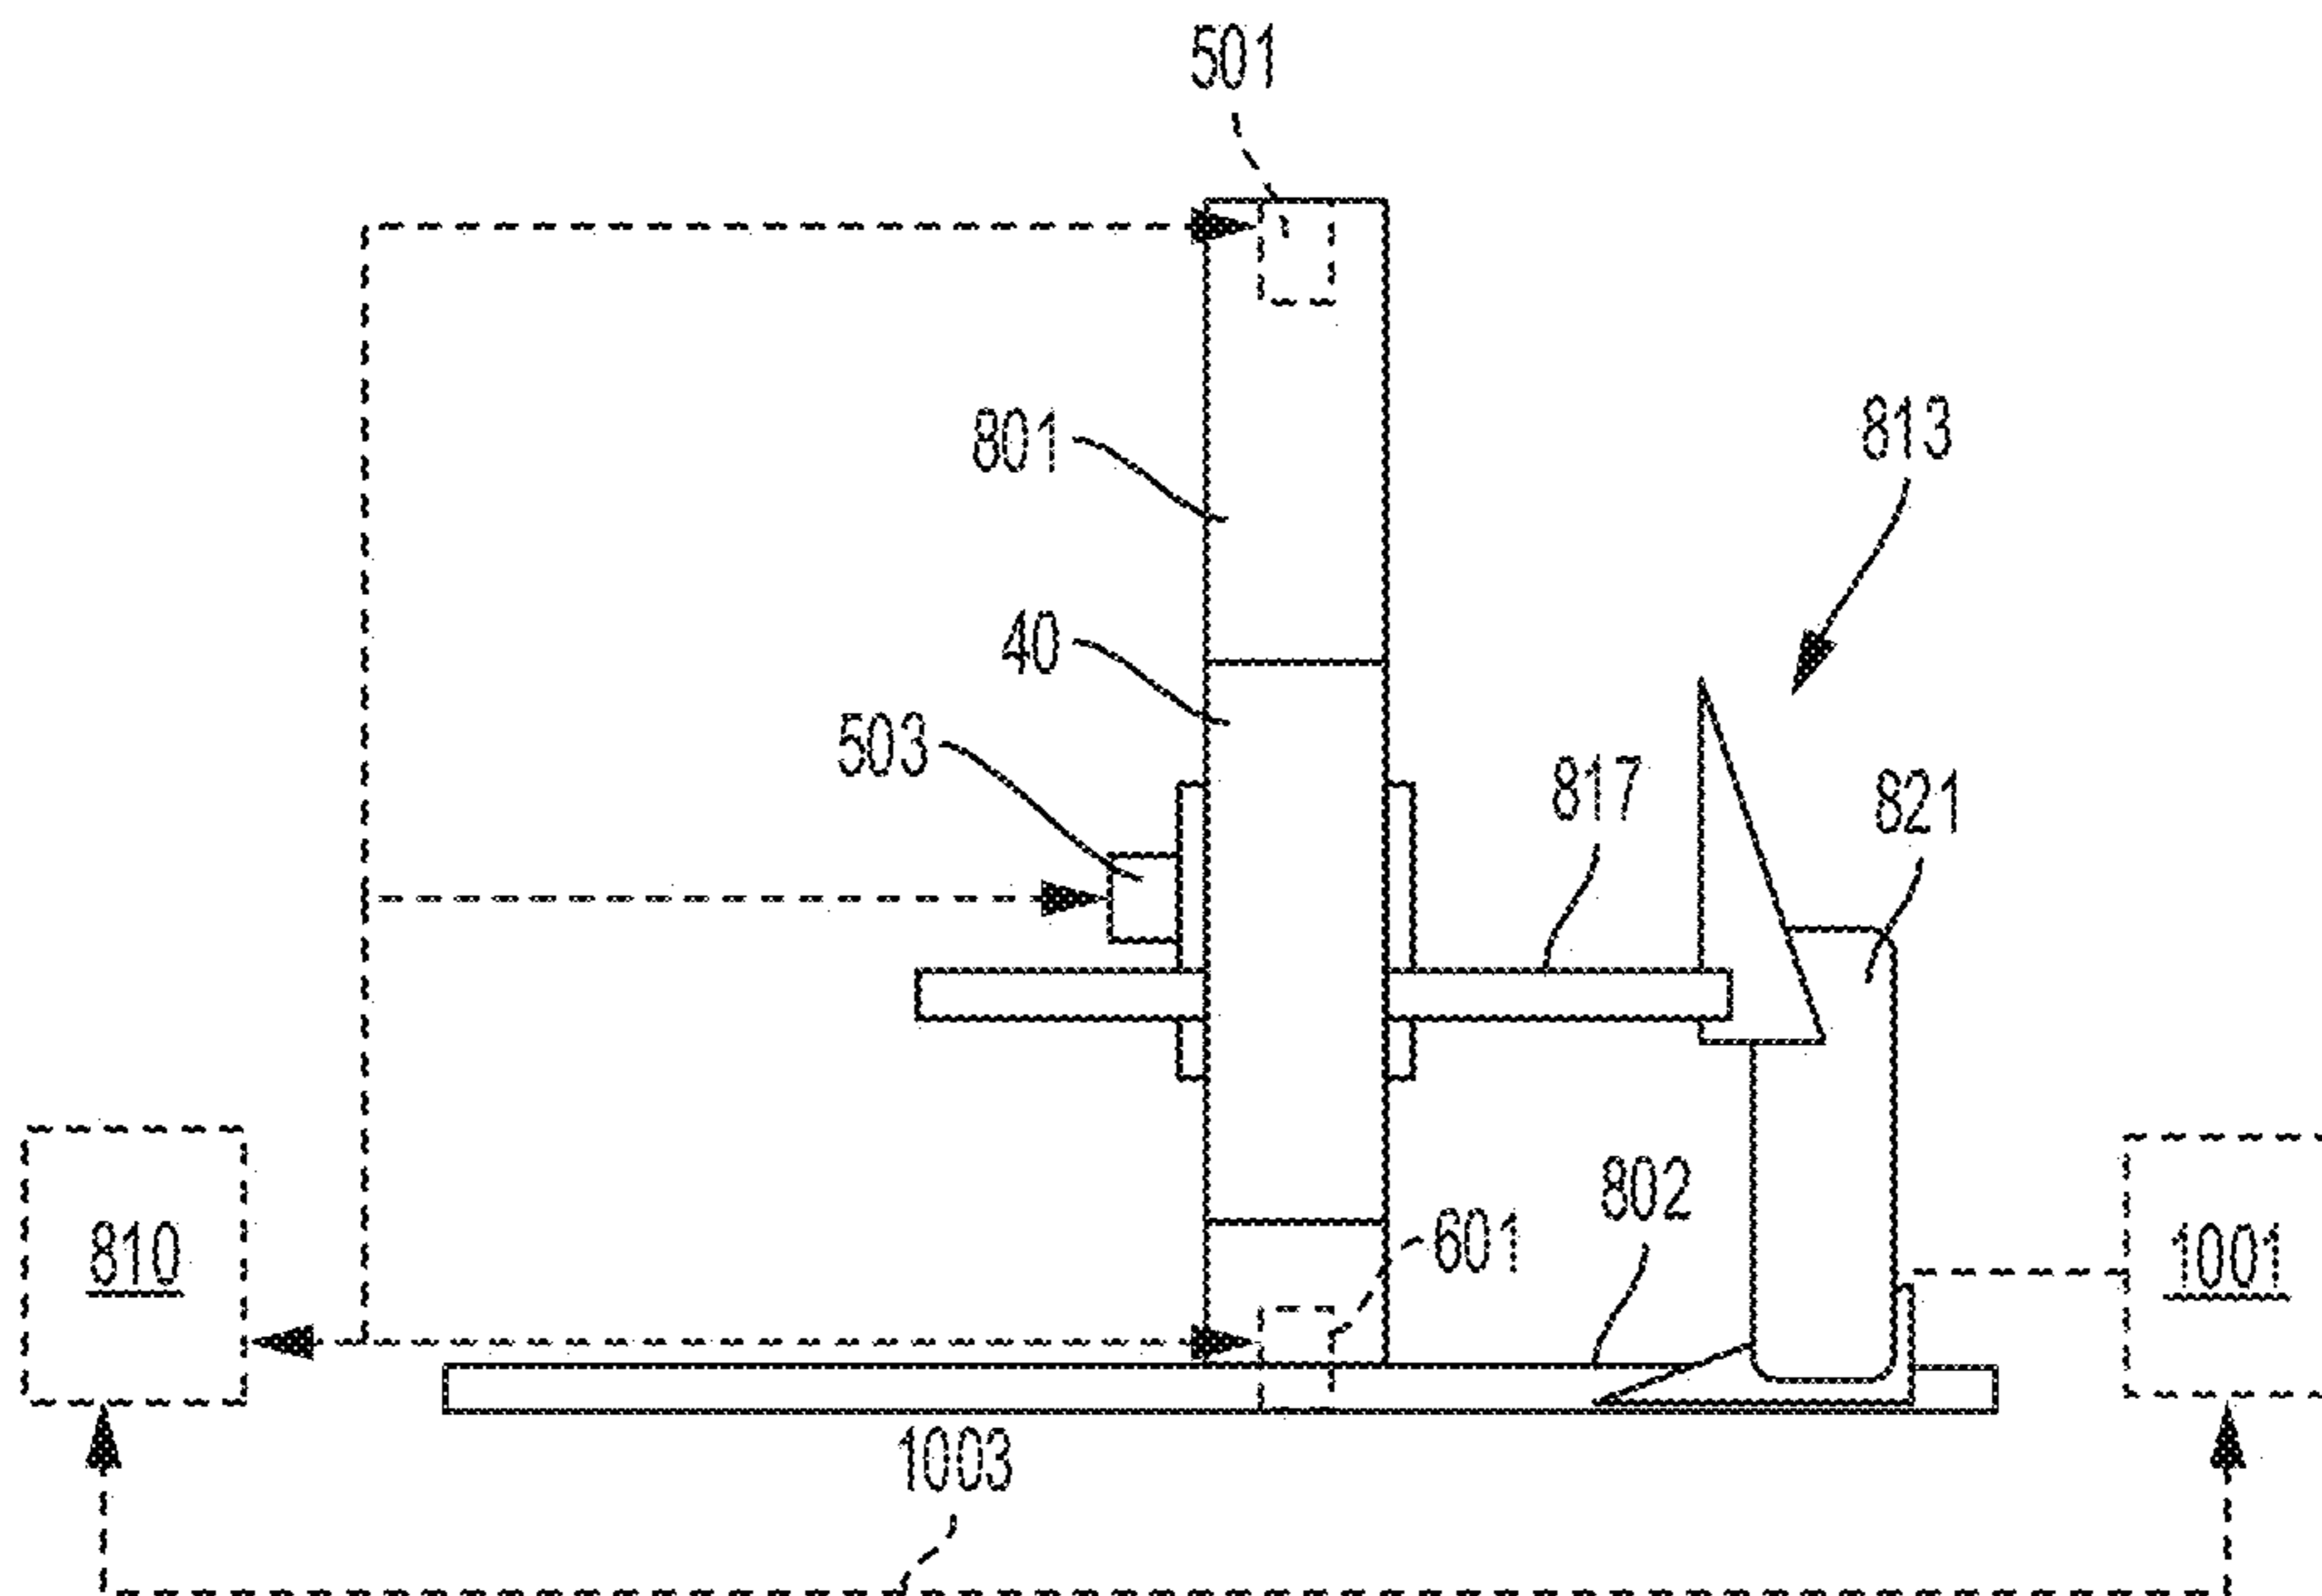


FIG. 10D

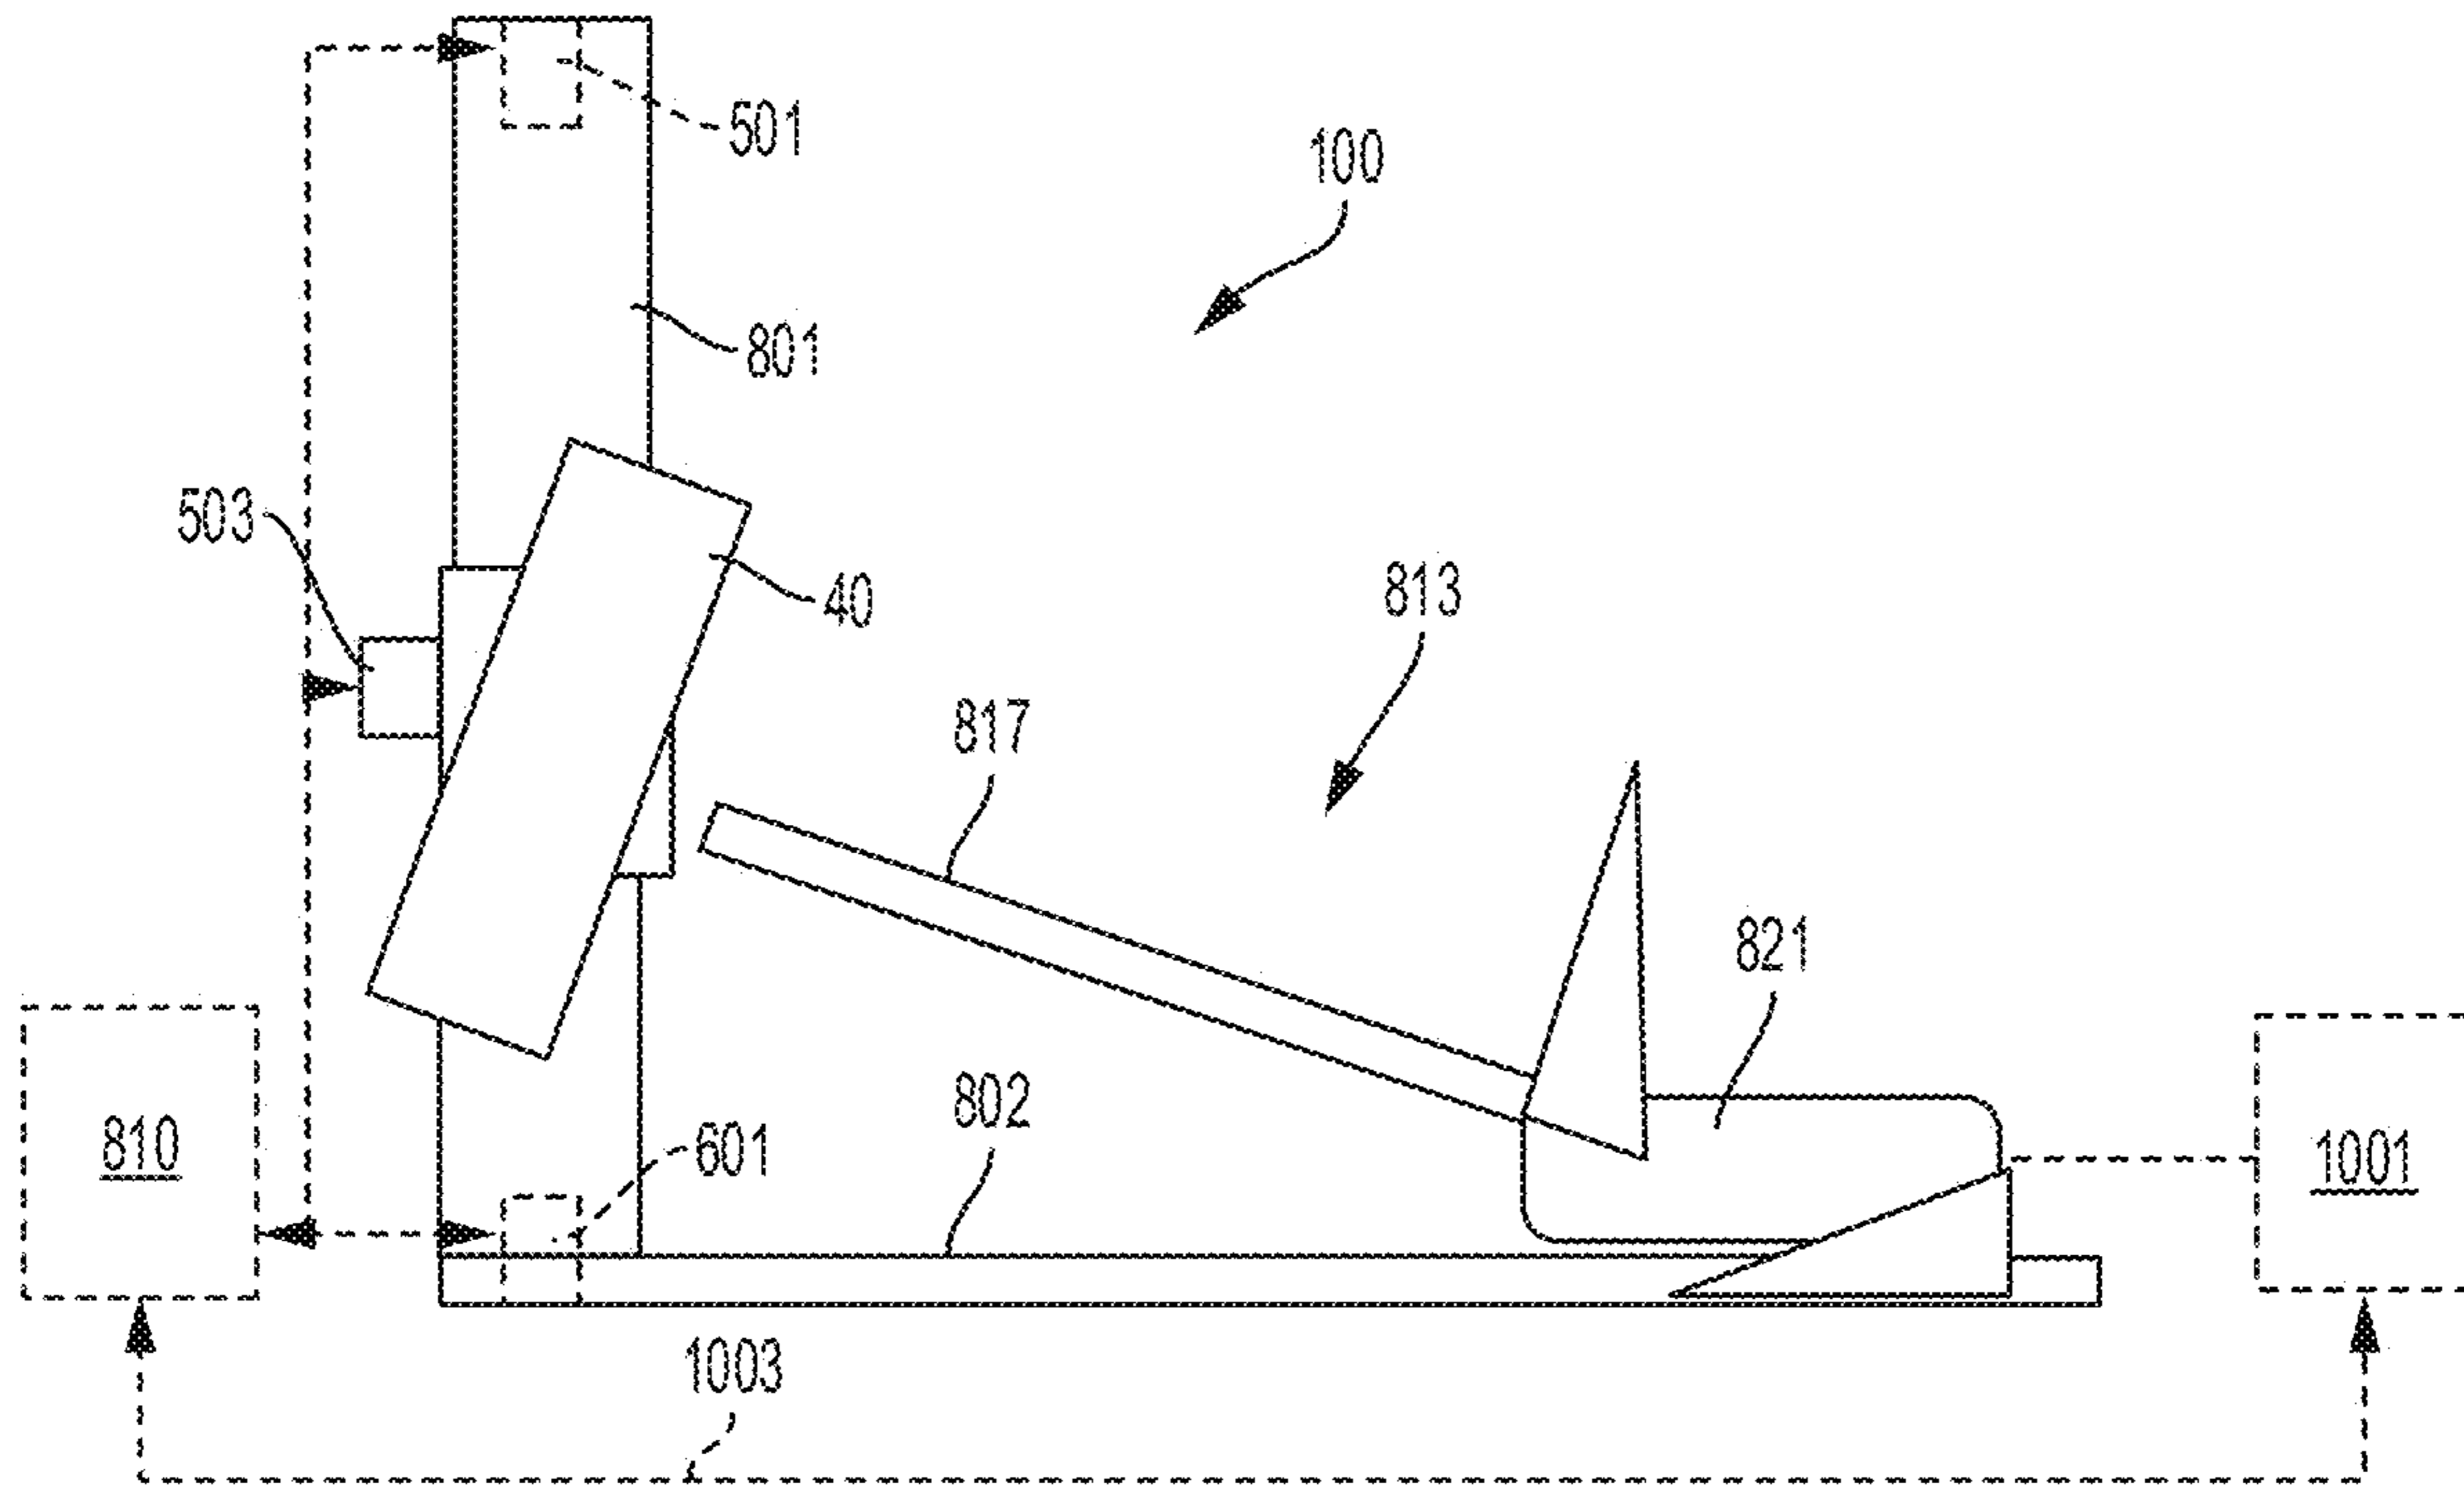


FIG. 10E

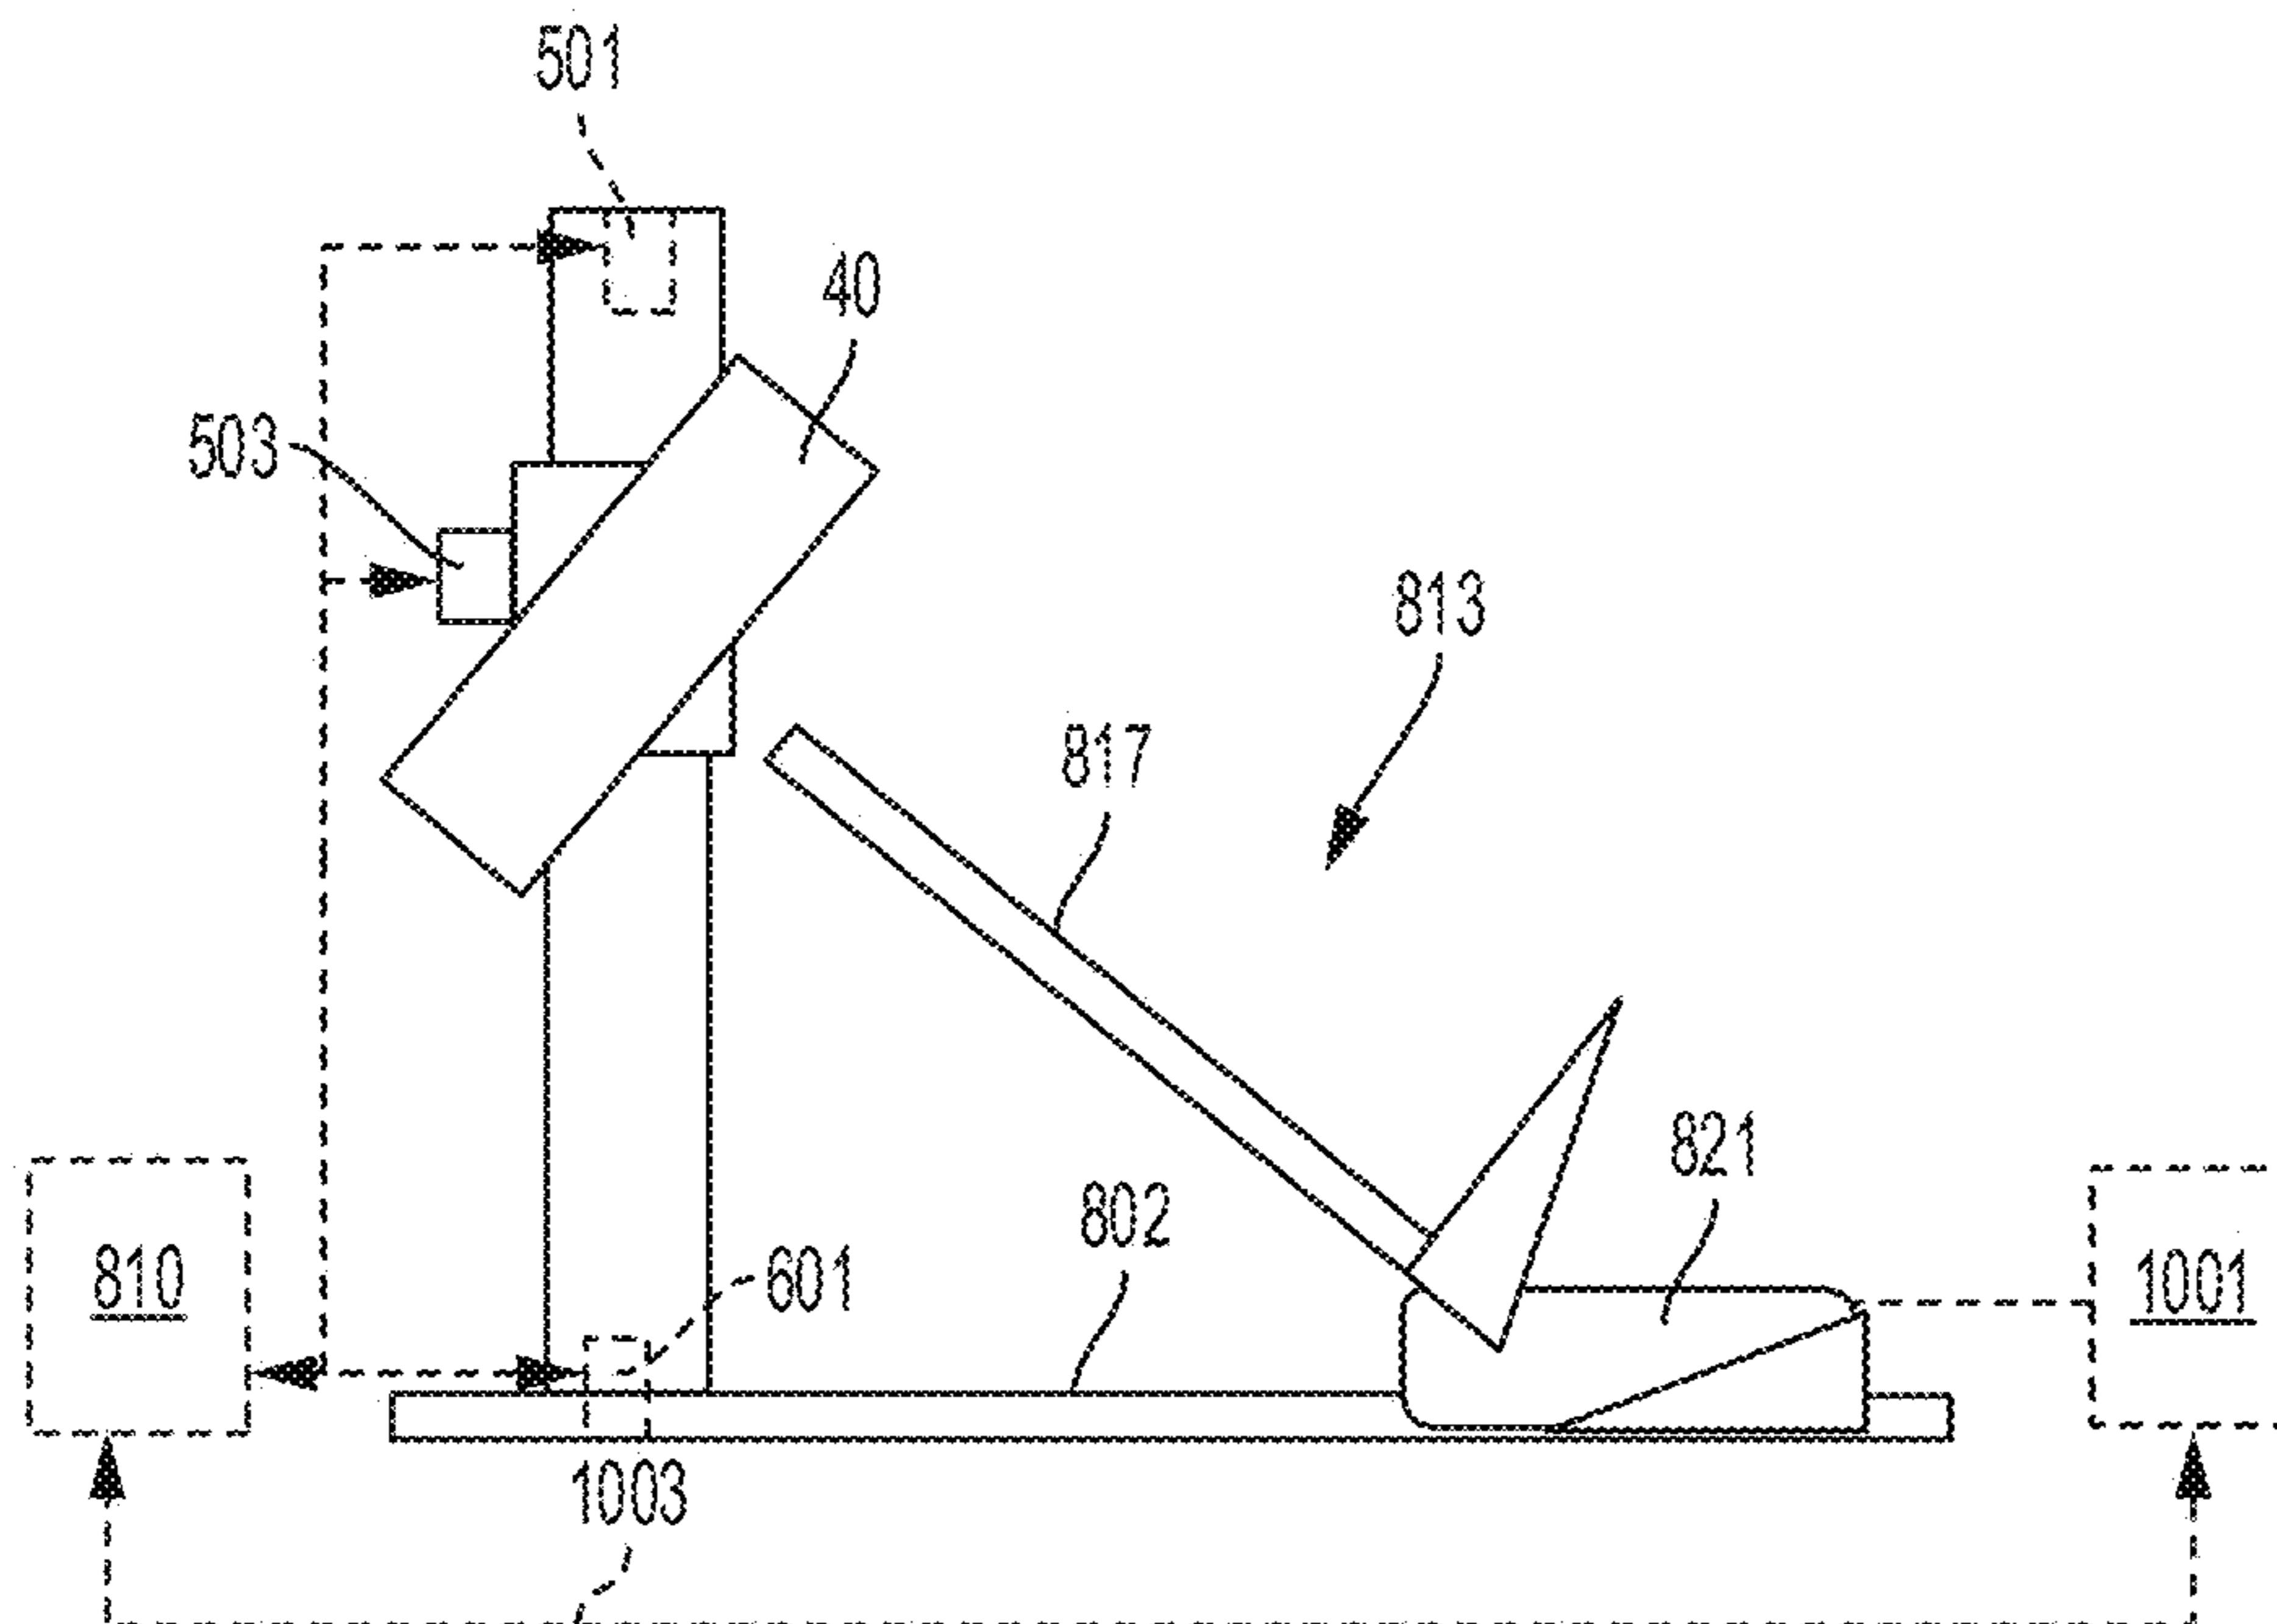


FIG. 10F

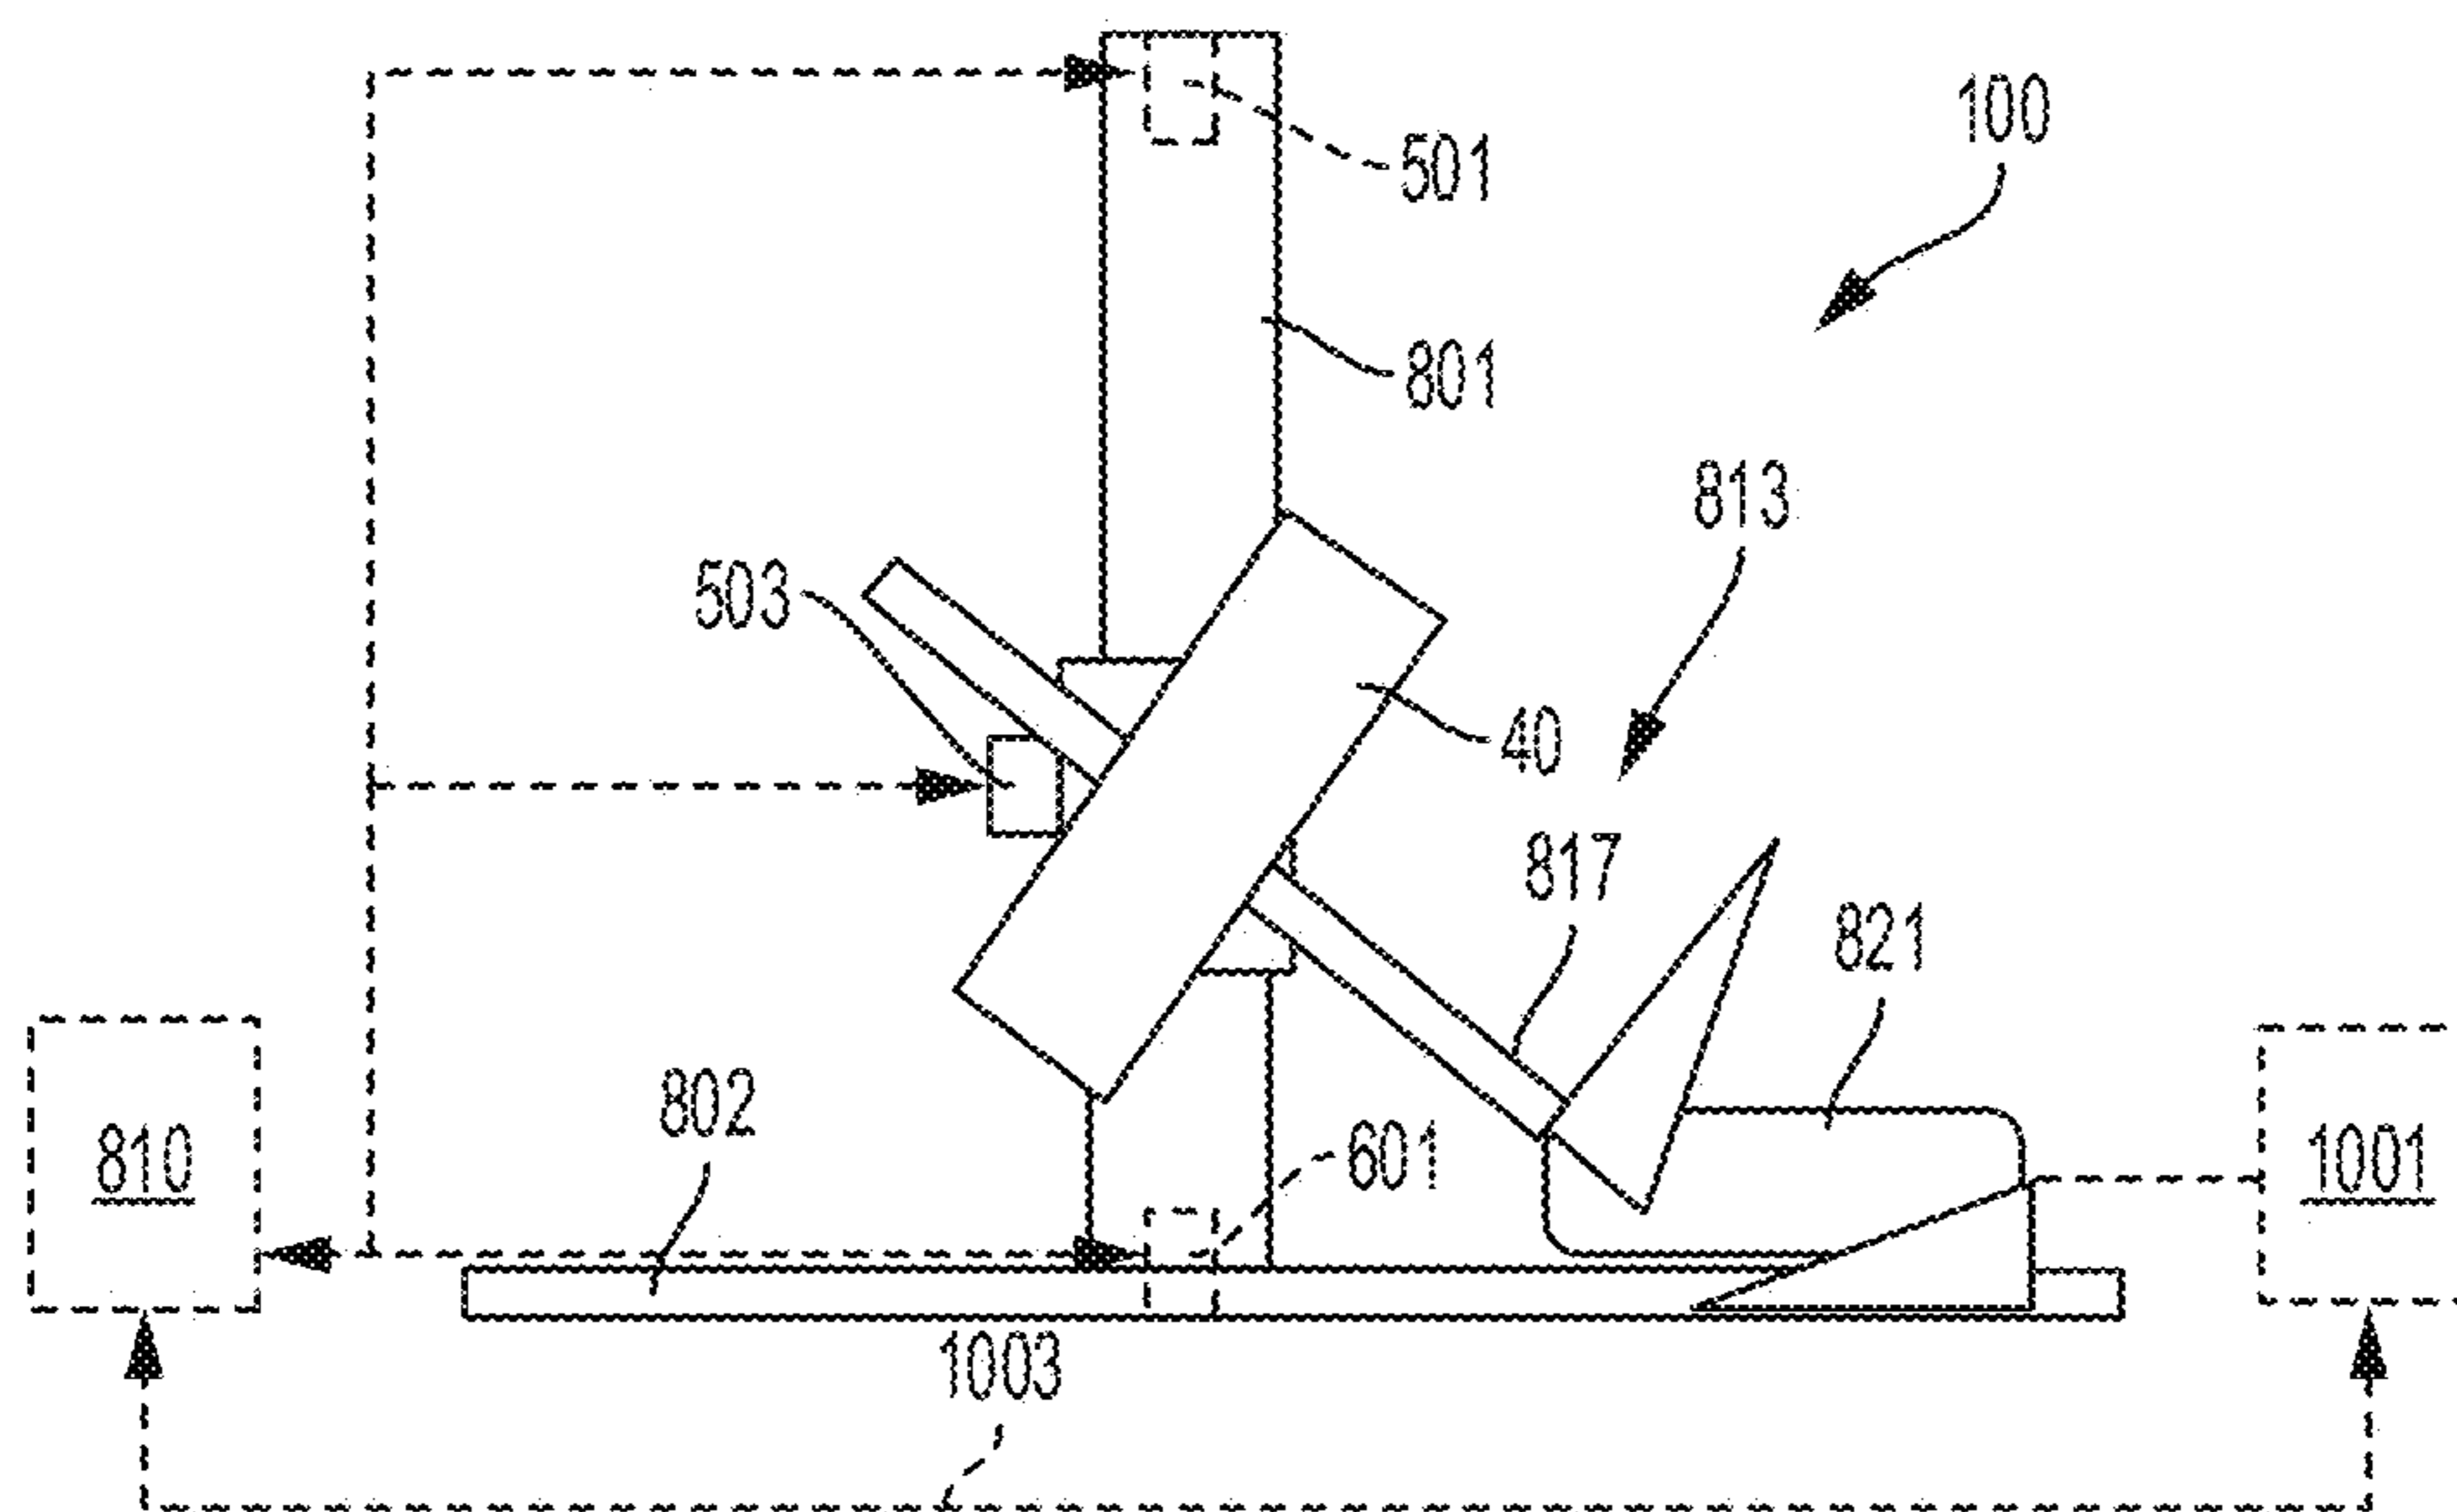


FIG. 10G

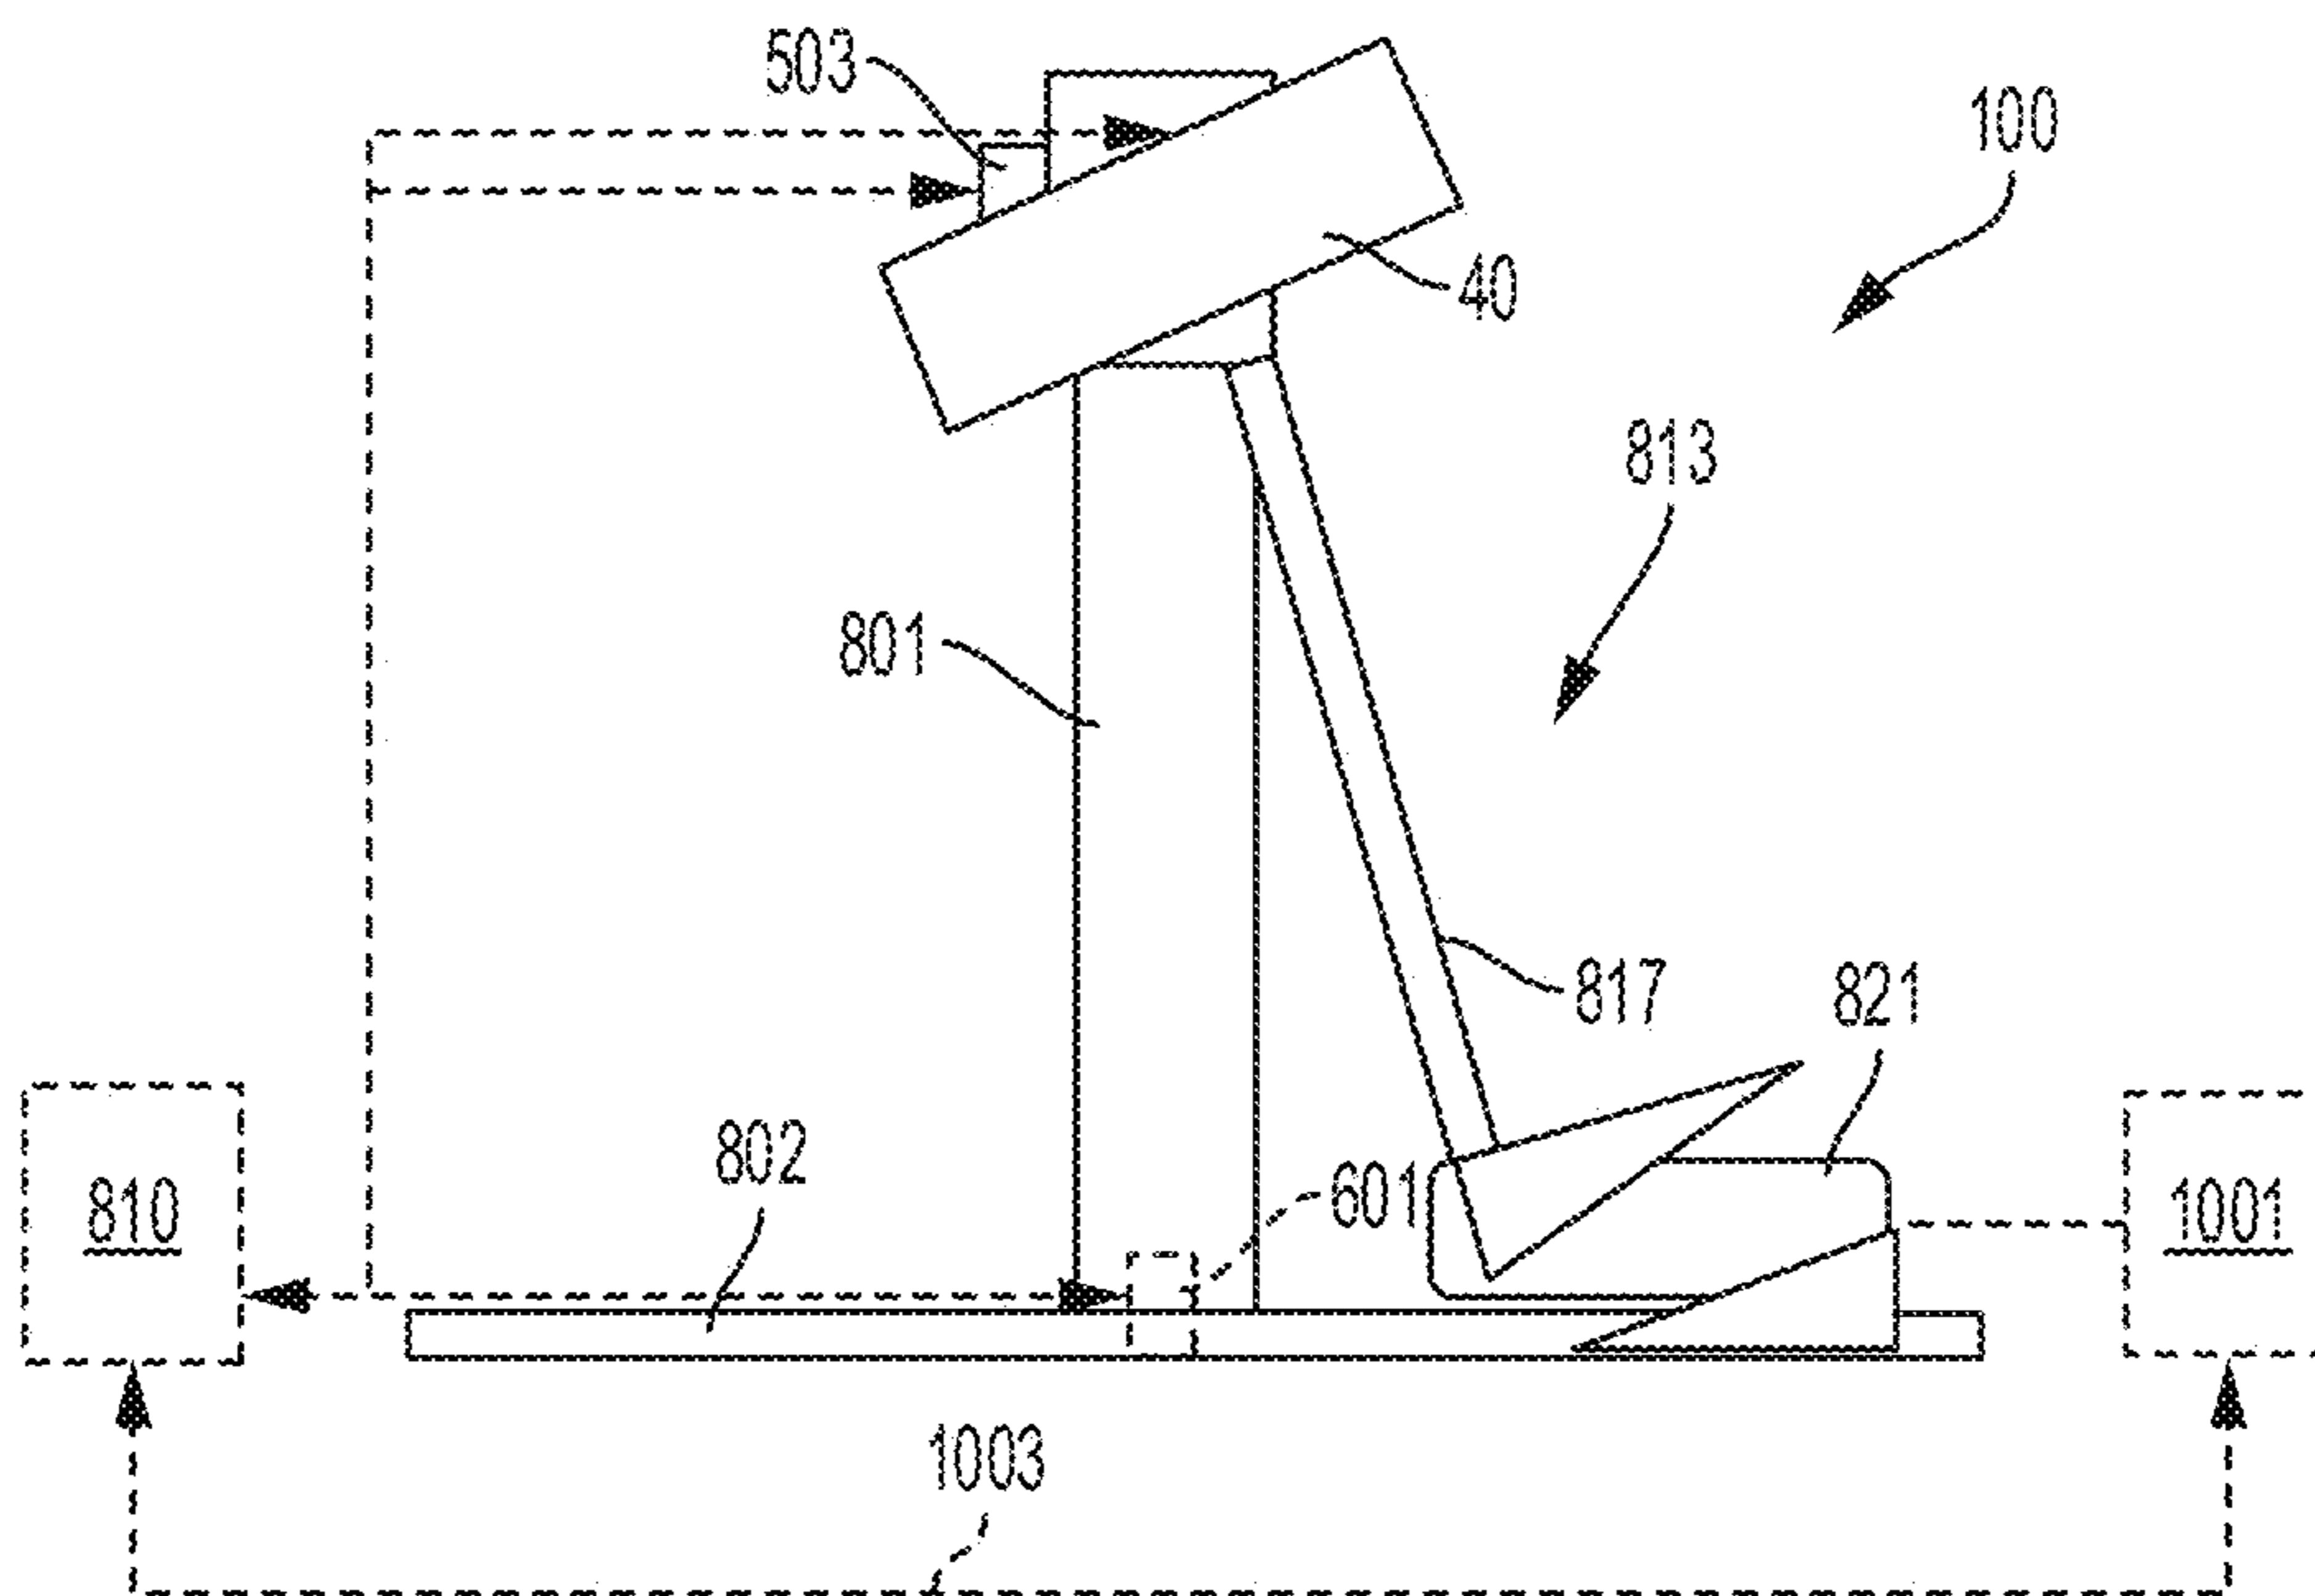


FIG. 10H

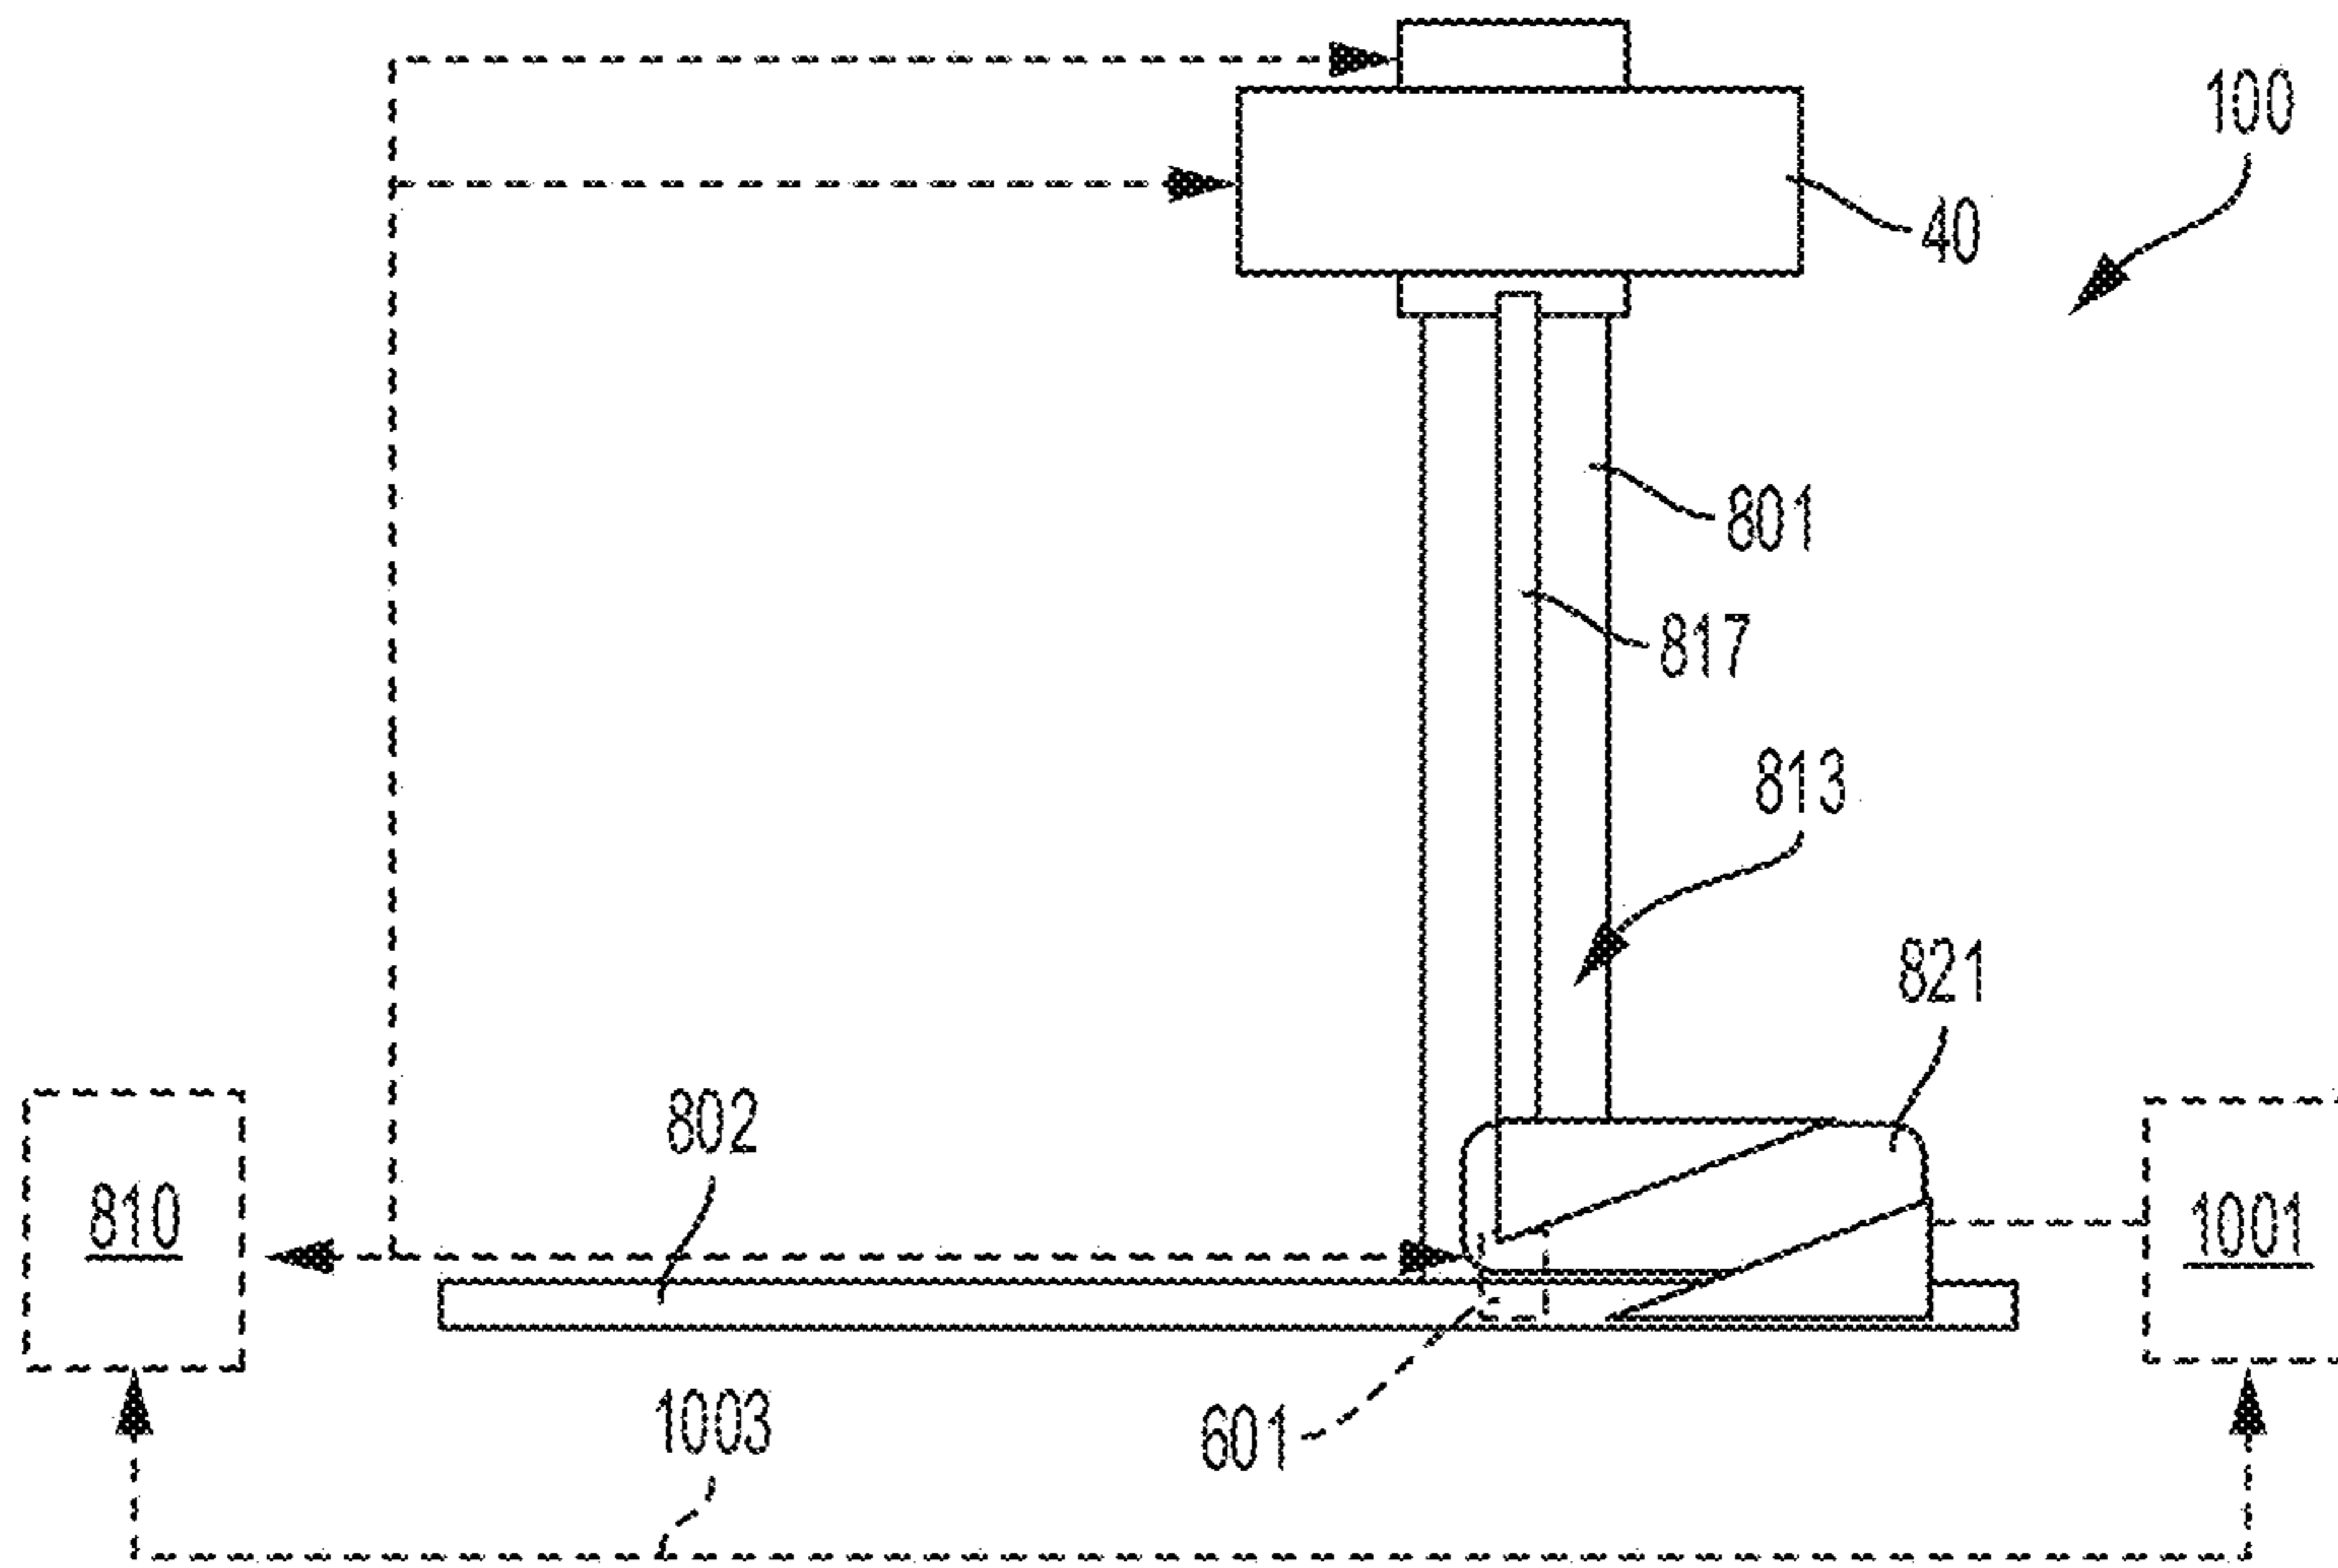


FIG. 10I

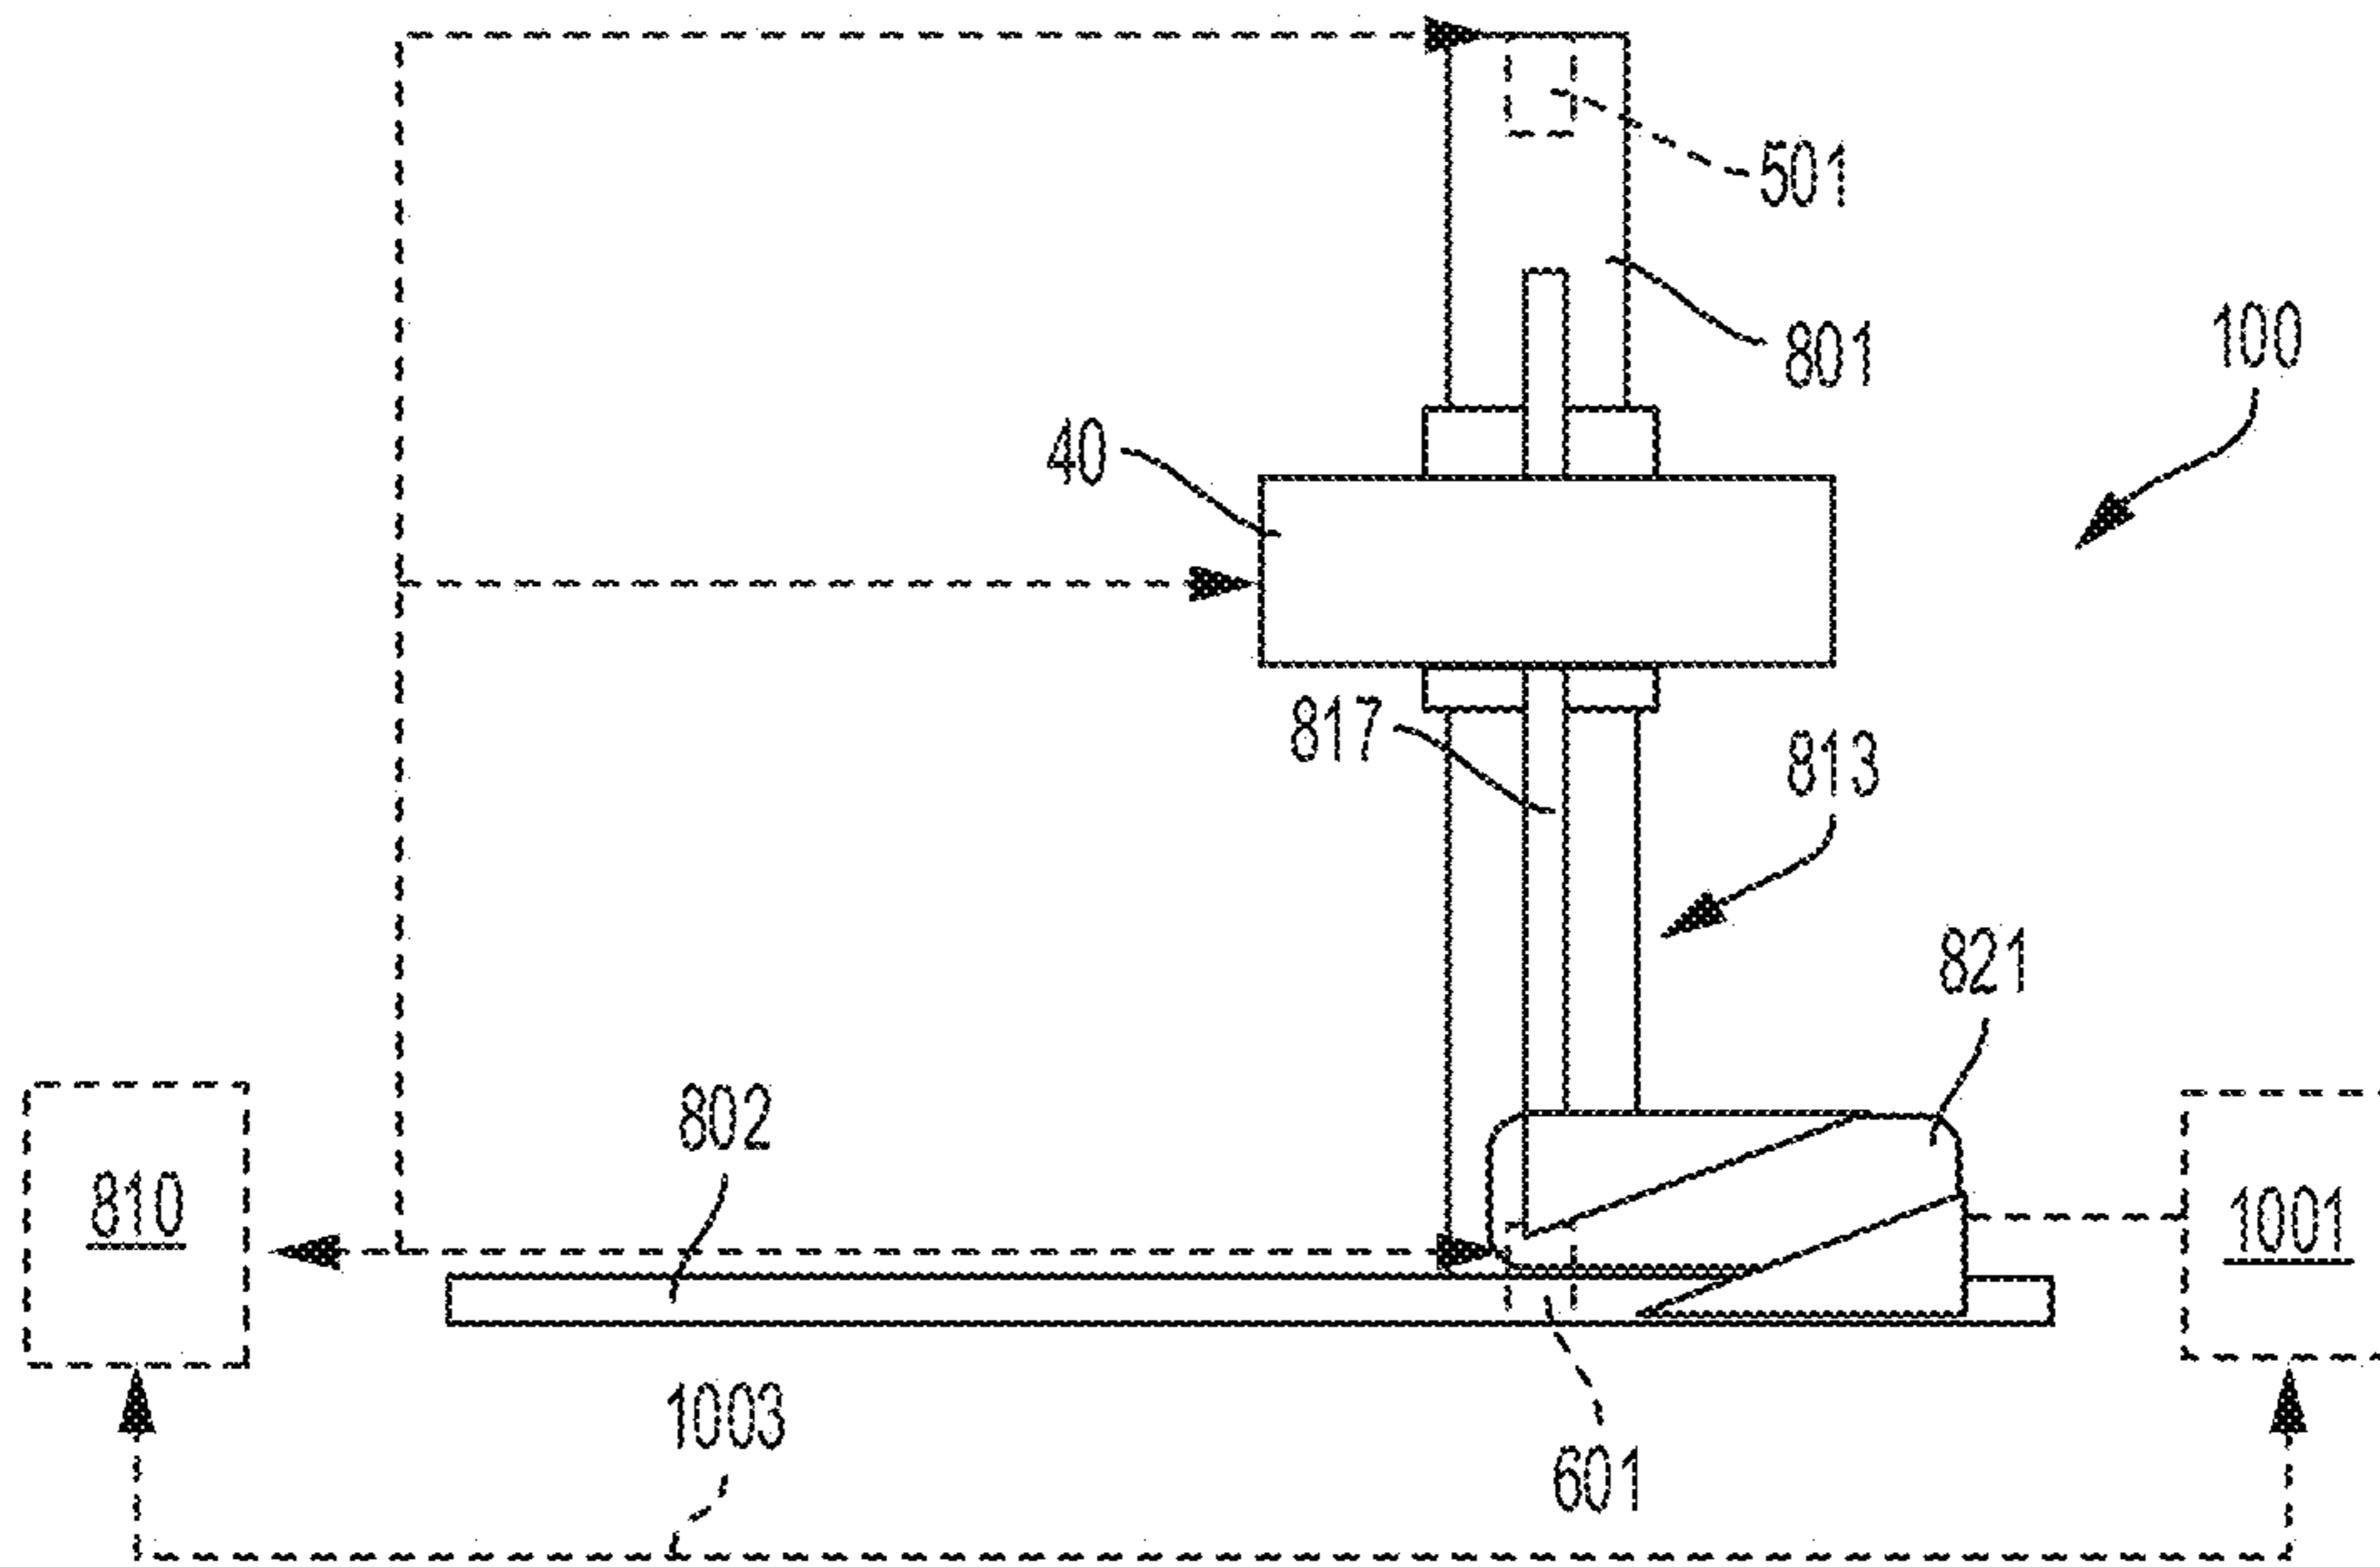


FIG. 10J

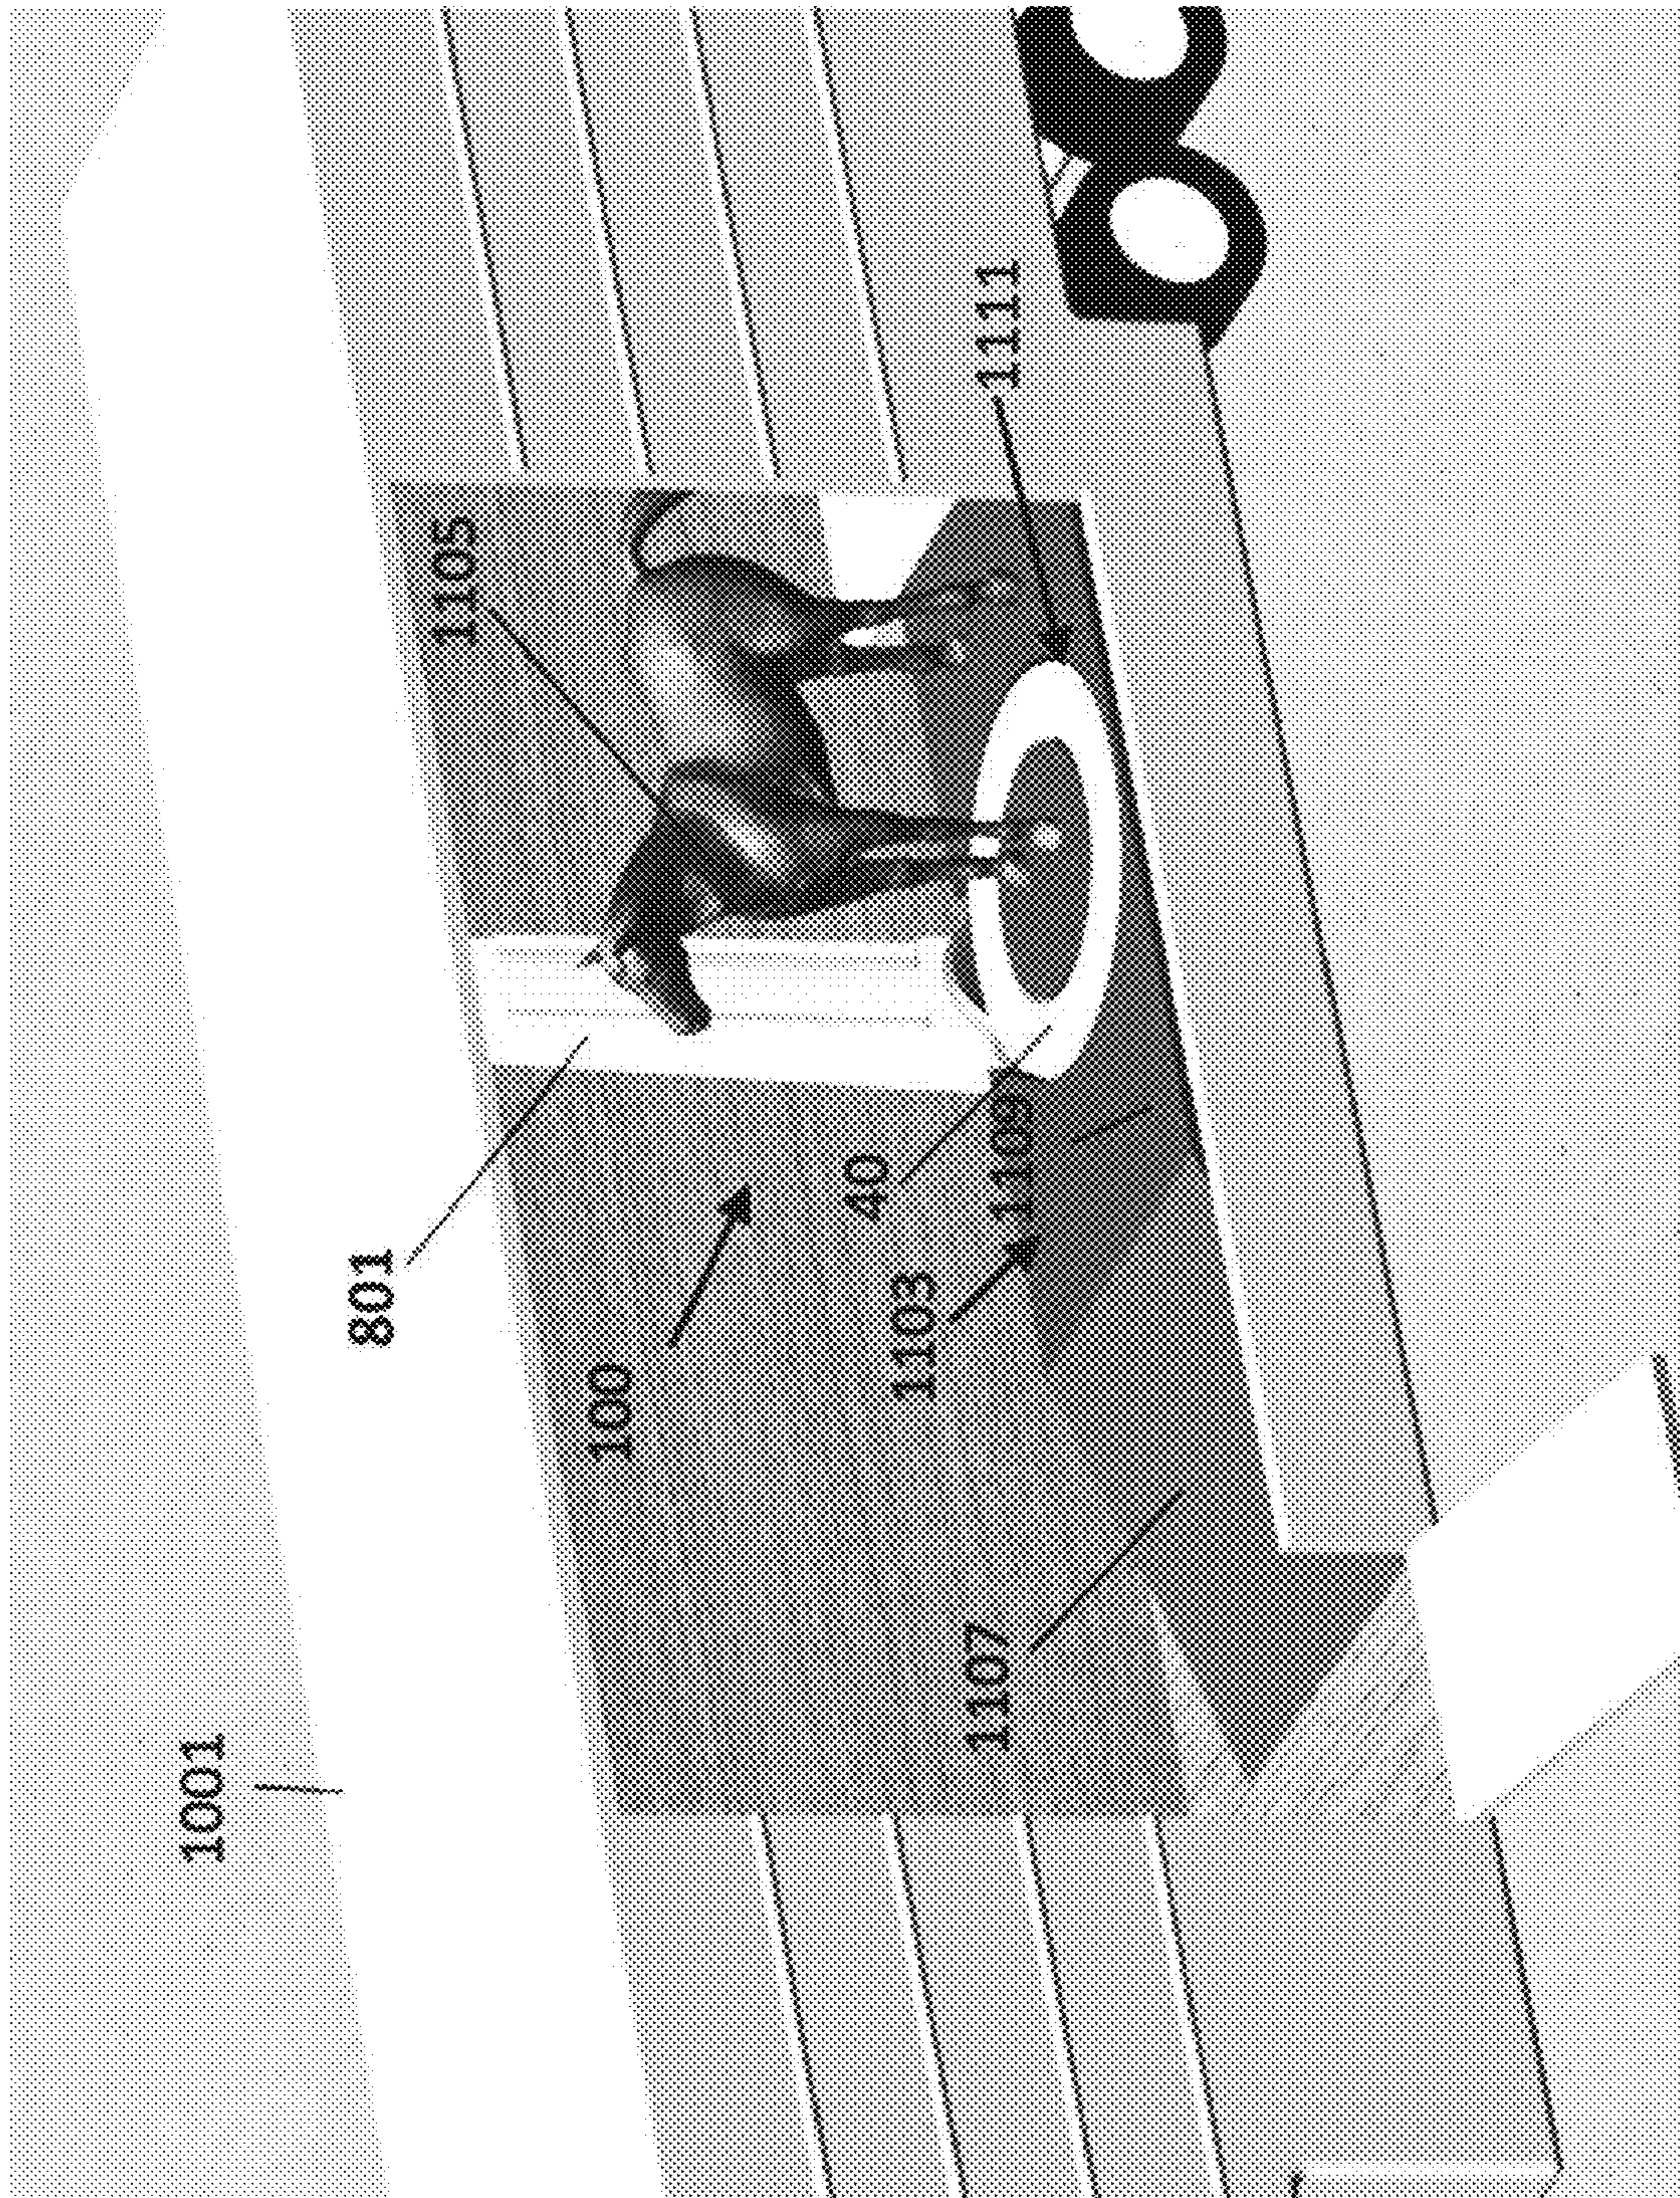


FIG. 11A

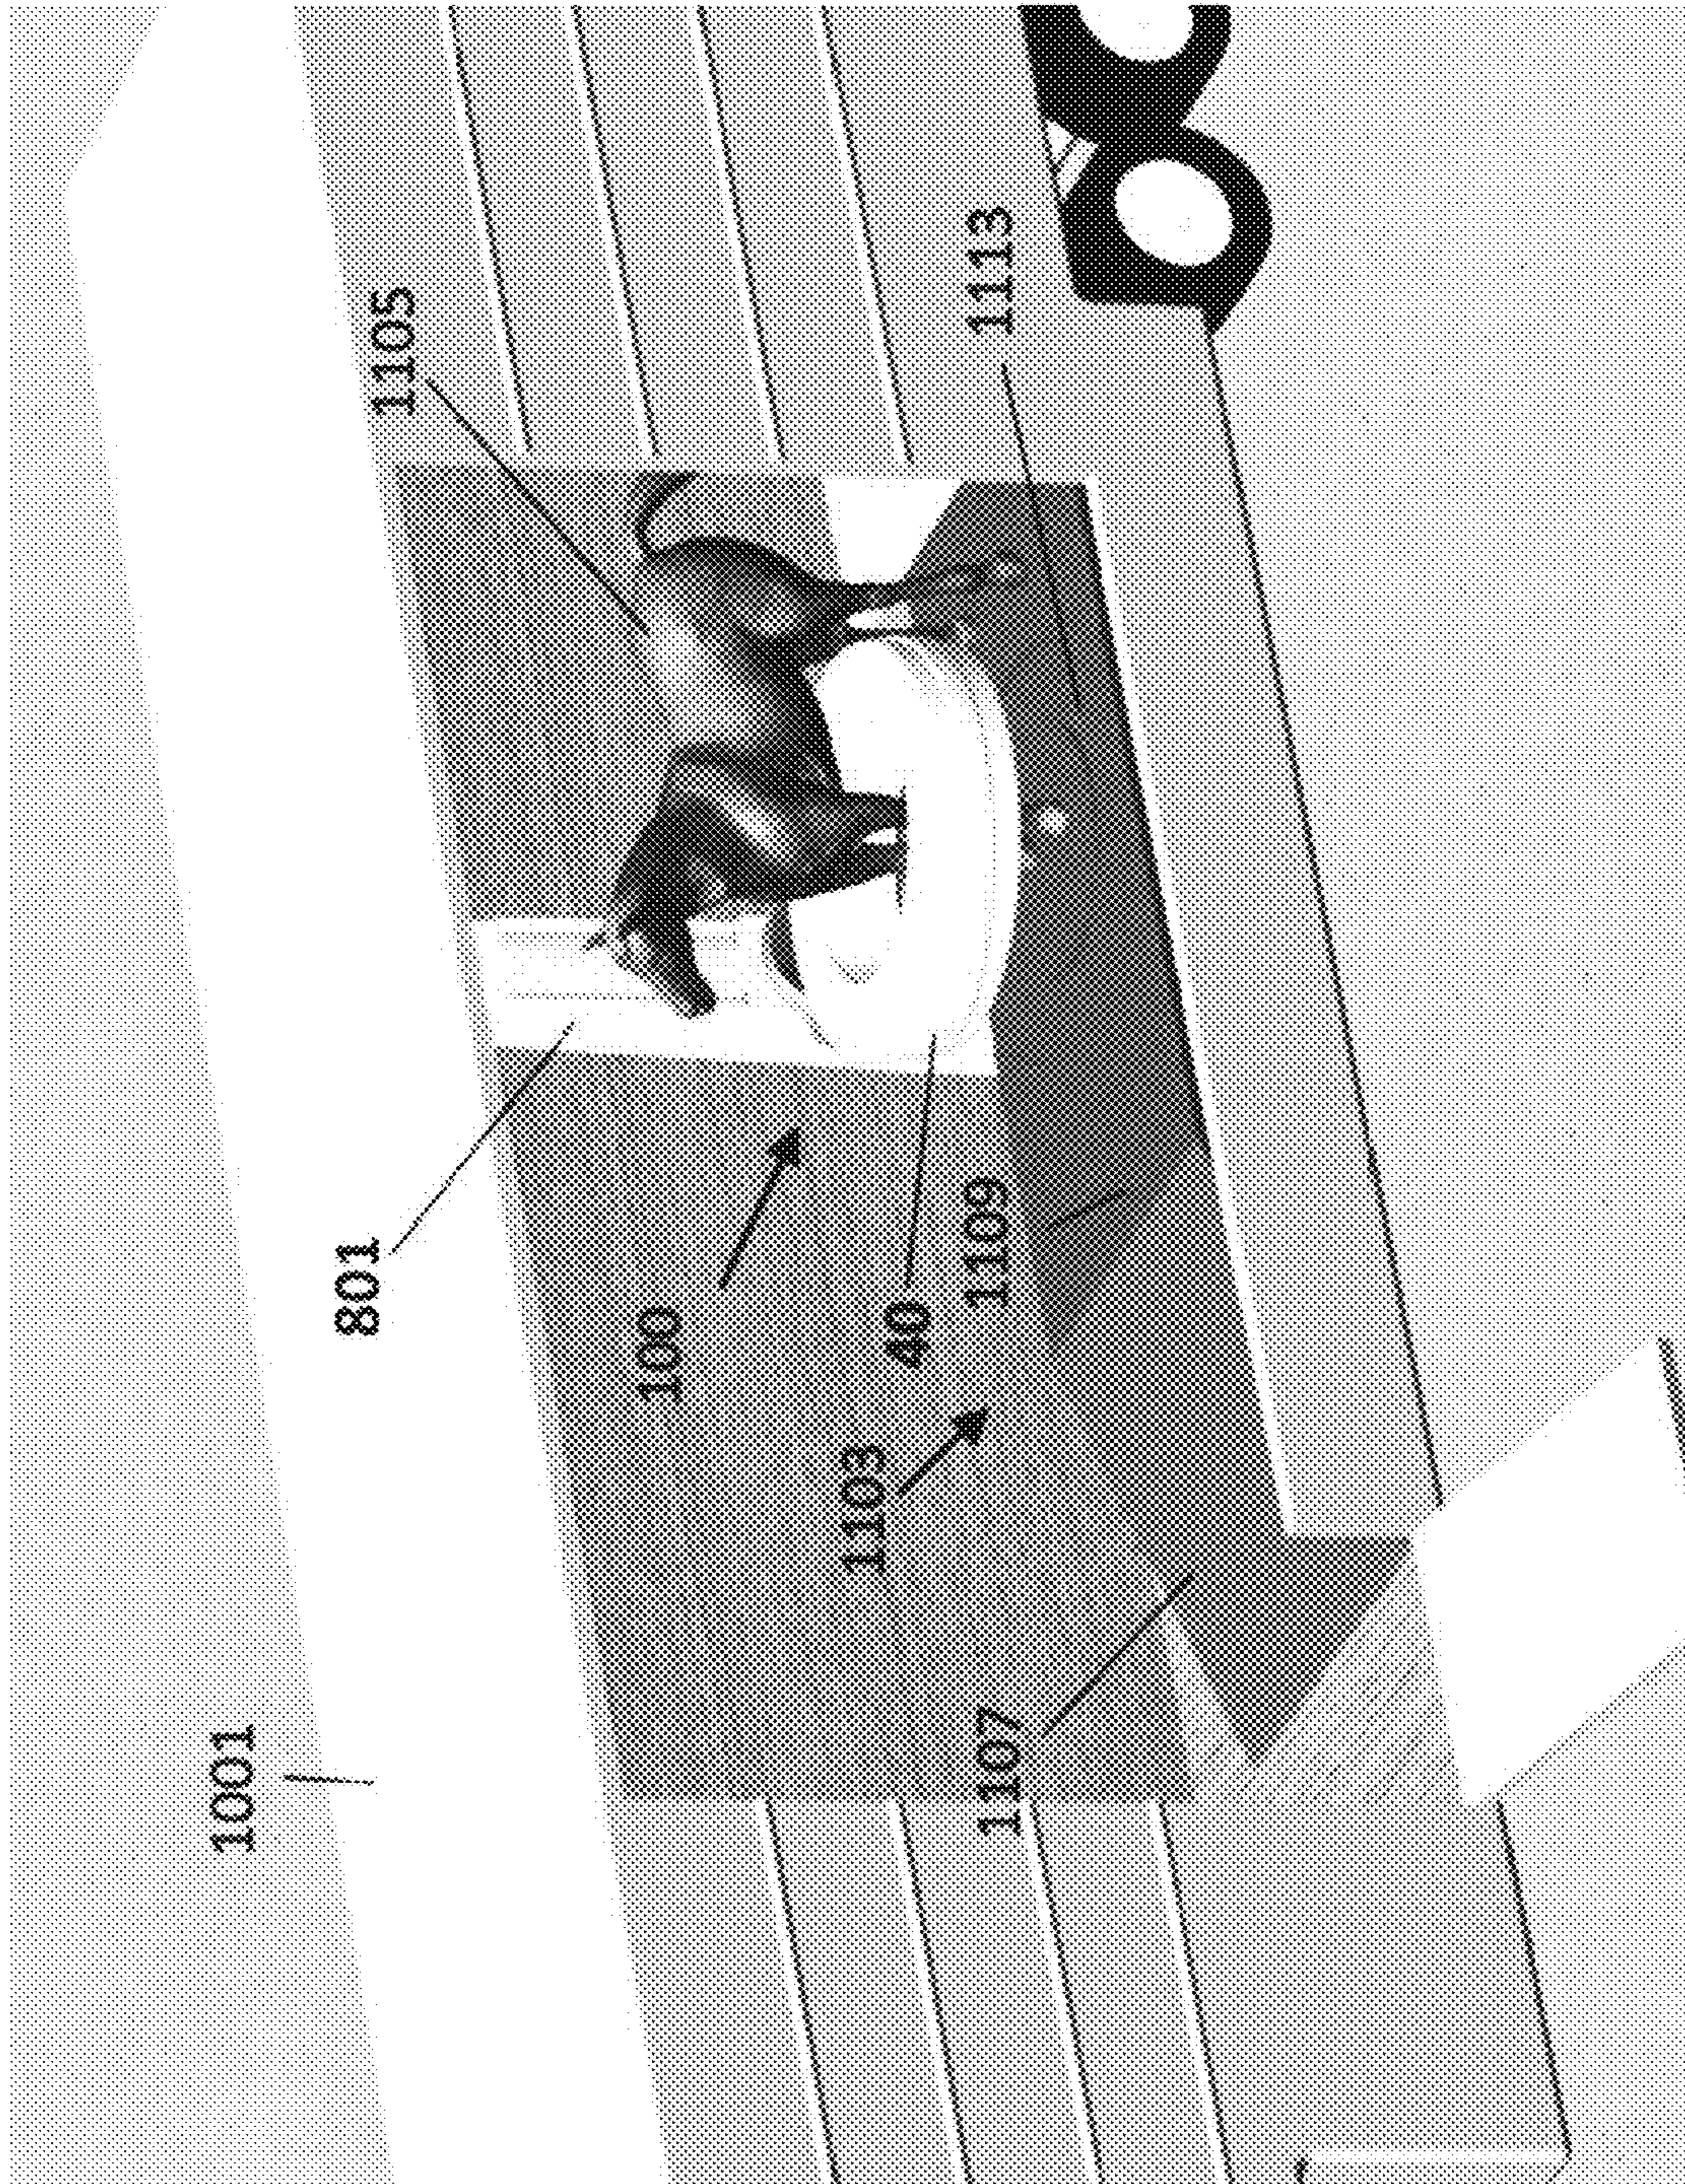


FIG. 11B

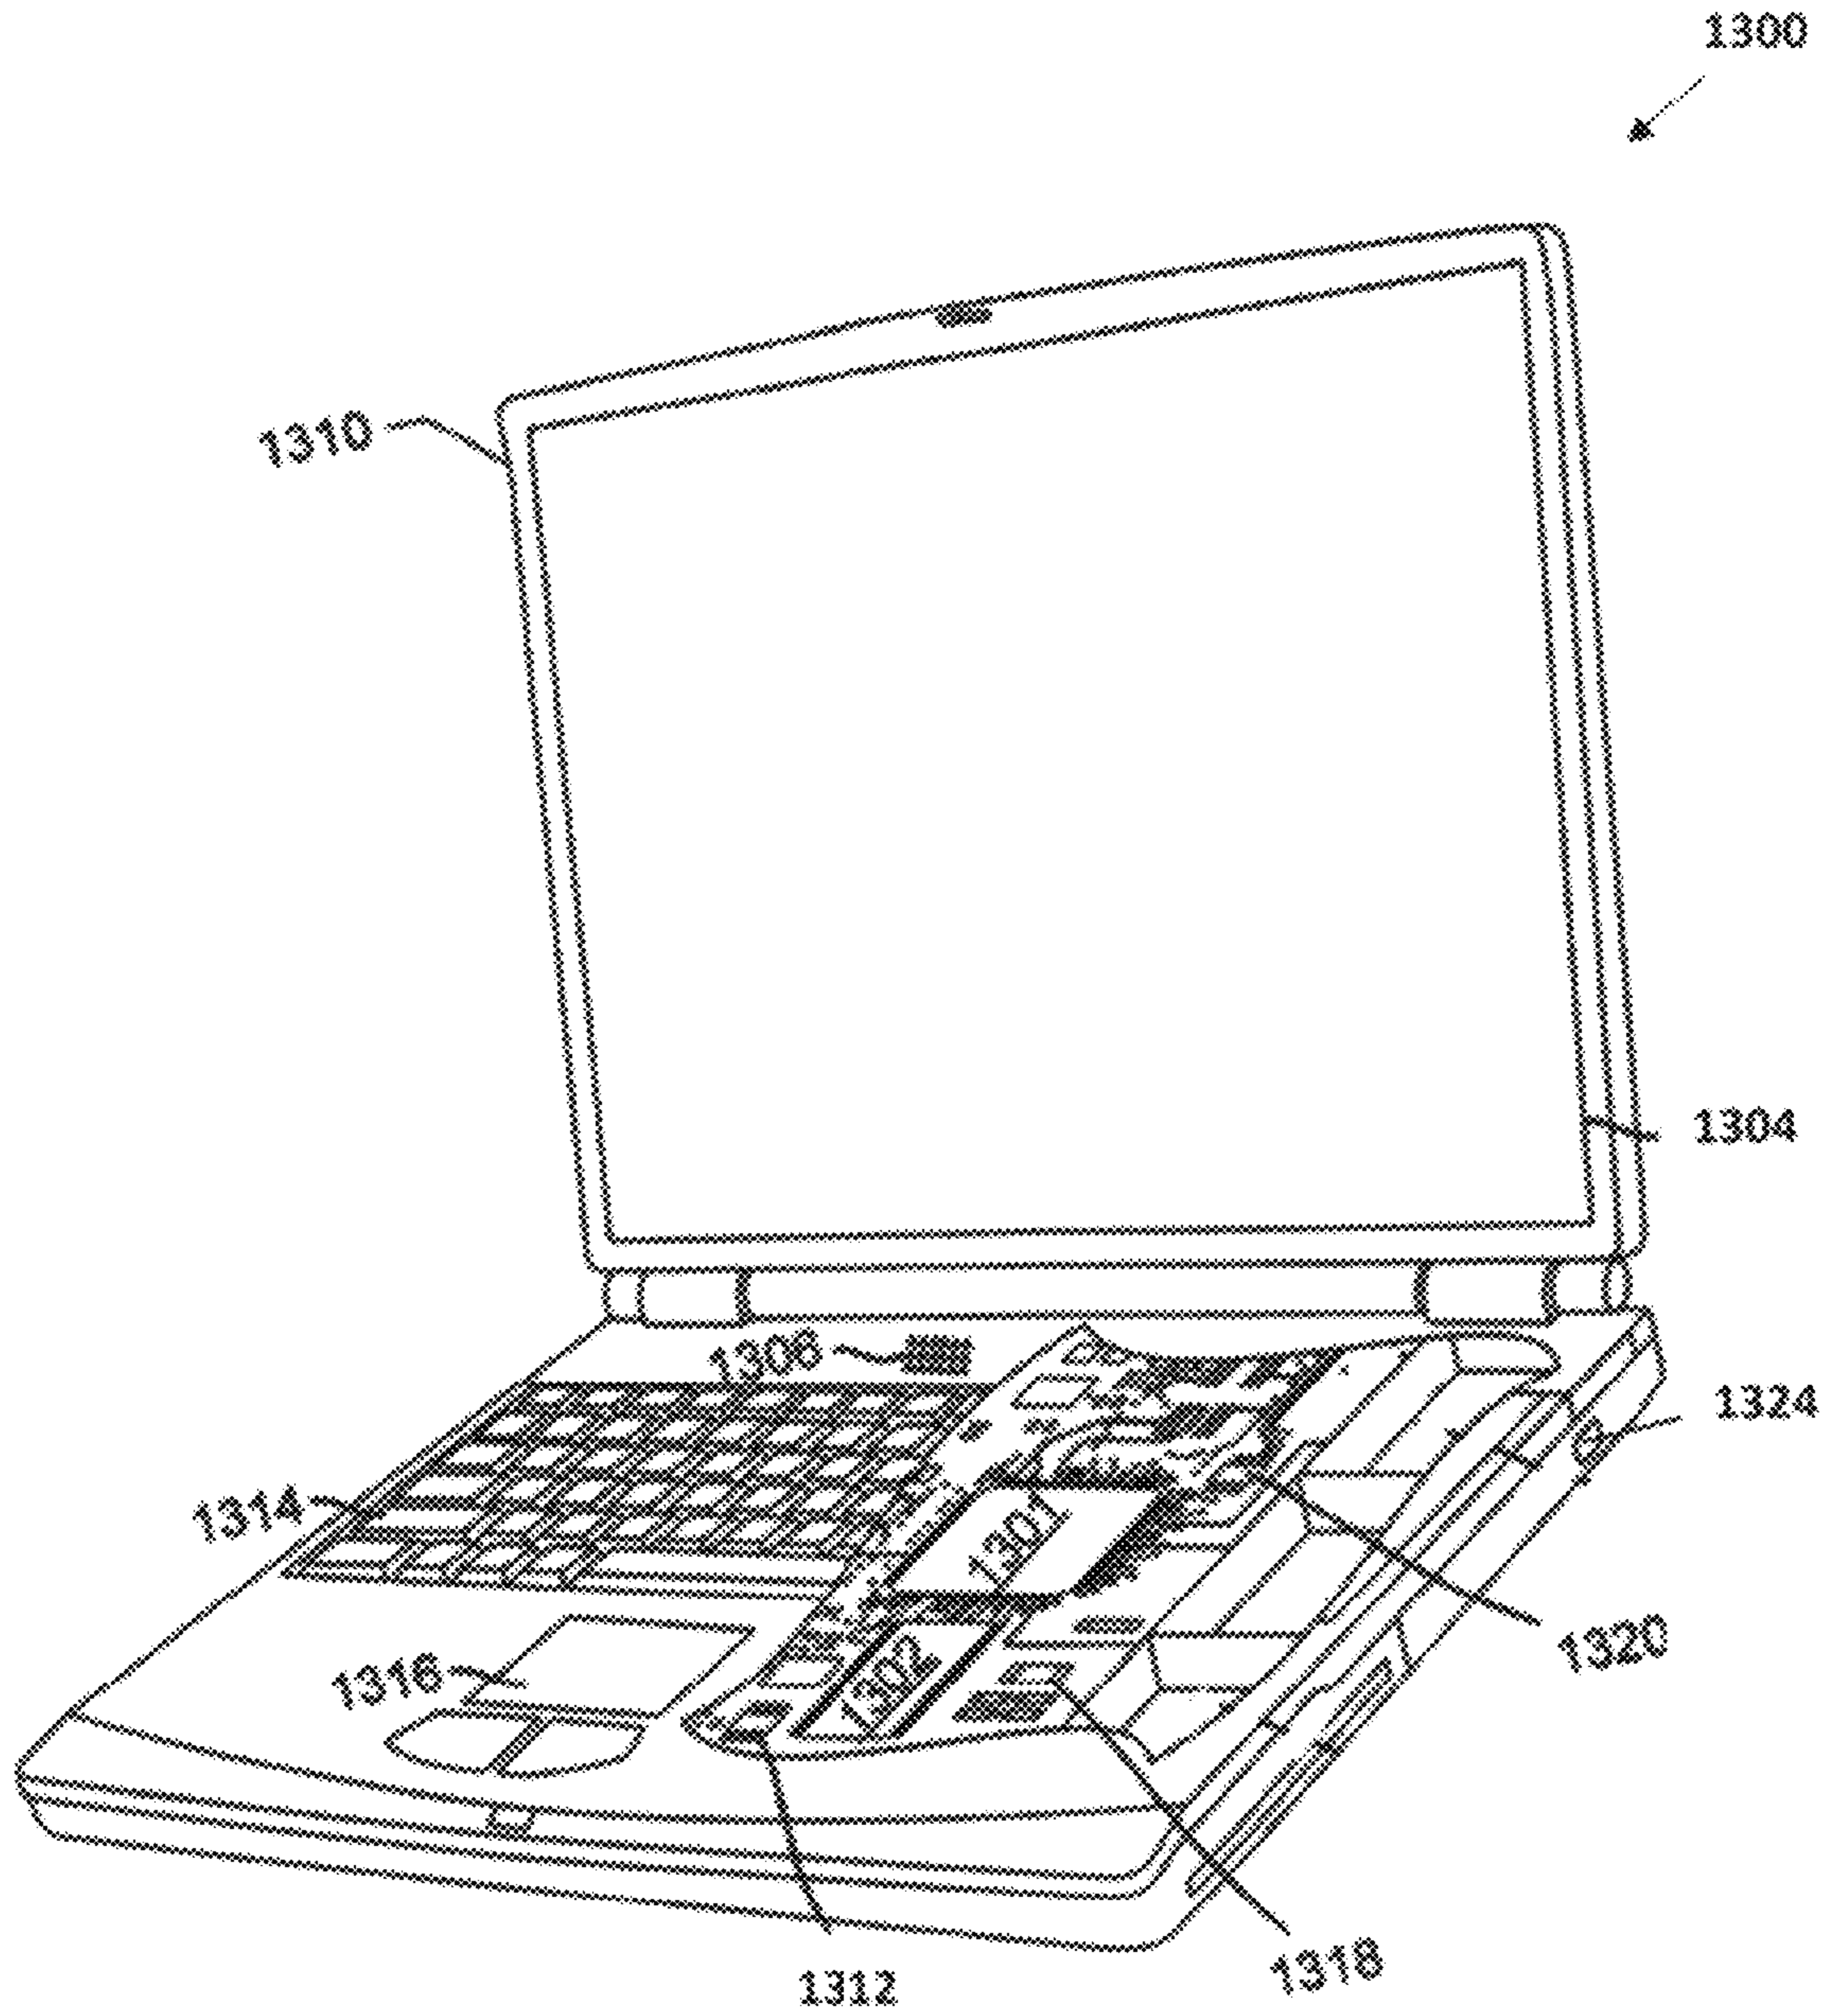


FIG. 12

CANTILEVERED X-RAY CT SYSTEM FOR MULTI-AXIS IMAGING

CROSS-REFERENCE TO RELATED APPLICATIONS

The subject application is a continuation of U.S. application Ser. No. 16/818,060, filed on Mar. 13, 2020, which is a continuation of U.S. application Ser. No. 15/817,672, filed on Nov. 20, 2017, which claims the benefit of priority to U.S. Provisional Application No. 62/425,746, filed on Nov. 23, 2016, the entire contents of each of which are incorporated herein by reference.

BACKGROUND

Conventional medical imaging devices, such as x-ray computed tomography (CT) imaging devices, are limited in the types of imaging operations that may be performed.

SUMMARY

Embodiments include a multi-axis imaging system and methods for imaging a human or animal using a multi-axis imaging system. The various embodiments include a multi-axis imaging system that includes an imaging gantry, a support column that supports the imaging gantry on one side of the gantry in a cantilevered manner, a base that supports the imaging gantry and the support column, a first drive mechanism that translates the gantry in a vertical direction relative to the support column, a second drive mechanism that rotates the gantry with respect to the support column, and a third drive mechanism that translates the support column and the gantry in a horizontal direction relative to the base.

Further embodiments include a method of operating a multi-axis imaging system comprising a moveable imaging gantry, the method including receiving, from a control system of a moveable patient support, data indicating the configuration of the patient support, and sending control signals to one or more drive systems of the multi-axis imaging system to cause the gantry to translate and/or rotate to maintain the gantry spaced away from the patient support and a bore of the gantry aligned with the patient support in response to the data received from the control system of the moveable patient support.

Further embodiments include a control system for a multi-axis imaging system having a moveable imaging gantry and a movable patient support, the control system including a memory and a processor configured with processor-executable instructions to perform operations including receiving data indicating a configuration of the movable patient support, and sending control signals to one or more drive systems of the multi-axis imaging system to cause the gantry to translate and/or rotate to maintain the gantry spaced away from the patient support and a bore of the gantry aligned with the patient support in response to the data received from the control system of the moveable patient support.

Further embodiments include a multi-axis imaging system for imaging an animal in a weight-bearing position that includes a gantry, a support column that supports the gantry, and a support stage on which an animal stands, wherein the gantry is translatable with respect to the support stage in a vertical direction to scan one or more legs of the animal standing on the support stage and the gantry is translatable in a vertical and in a horizontal direction with respect to the

support stage to scan a head and/or neck of the animal standing on the support stage.

BRIEF DESCRIPTION OF THE DRAWINGS

Other features and advantages of the present invention will be apparent from the following detailed description of the invention, taken in conjunction with the accompanying drawings of which:

FIG. 1 illustrates a multi-axis CT imaging device according to an embodiment.

FIGS. 2A-2C illustrate a multi-axis x-ray CT imaging device performing a scan of a patient in a vertical direction.

FIGS. 3A-3C illustrate the multi-axis x-ray CT imaging device performing a scan of a patient in a horizontal direction.

FIGS. 4A-4C illustrate the multi-axis x-ray CT imaging device performing a scan of a patient in an oblique direction.

FIGS. 5A-5D illustrate a vertical support column for an x-ray gantry according to an embodiment.

FIGS. 6A-6B illustrate a base of an x-ray CT imaging system according to an embodiment.

FIG. 7A-7E illustrate a gantry and a bearing assembly for a multi-axis imaging system according to an embodiment.

FIG. 8 schematically illustrates a bearing assembly attached to a gantry shell according to an embodiment.

FIG. 9 illustrates components mounted to a rotor according to an embodiment.

FIGS. 10A-10K illustrate methods of operating a multi-axis imaging system and moveable patient support to perform an imaging scan of a patient.

FIGS. 11A-11C illustrate a multi-axis imaging system for imaging an animal in a standing position.

FIG. 12 schematically illustrates a computing device which may be used for performing various embodiments.

DETAILED DESCRIPTION

The various embodiments will be described in detail with reference to the accompanying drawings. Wherever possible, the same reference numbers will be used throughout the drawings to refer to the same or like parts. References made to particular examples and implementations are for illustrative purposes, and are not intended to limit the scope of the invention or the claims.

Referring to FIG. 1, an imaging system 100 according to one embodiment of the invention is shown. The system 100 includes image collection components, such as a rotating x-ray source and detector array, a rotating gamma-ray camera or stationary magnetic resonance imaging components, that are housed within the gantry 40. The system 100 is configured to collect imaging data, such as, for example x-ray computed tomography (CT), positron emission tomography (PET), single-photon emission computed tomography (SPECT) or magnetic resonance imaging (MRI) data, from an object located within the bore 116 of the gantry 40, in any manner known in the medical imaging field. In embodiments, the system 100 may be an x-ray CT imaging system, and may include an x-ray source and a detector located within the gantry 40. The gantry 40 may also include other components, such as a high-voltage generator, a heat exchanger, a power supply (e.g., battery system), and a computer. These components may be mounted on a rotating element (e.g., a rotor) that rotates within the gantry 40 during an imaging scan. A rotor drive mechanism may also be located on the rotor, and may drive the rotation of the rotor. Between scans, a docking system may be used to

couple the rotating and non-rotating portions of the system 100 for power and data communication.

The gantry 40 may be mounted to a support column 801. The support column 801 may be attached to the gantry 40 on a first side of the gantry 40 and may support the gantry 40 in a cantilevered manner. The gantry 40 may be a generally O-shaped structure having a central imaging bore 116 and defining an imaging axis 114 extending through the bore. The system 800 may also include a base 802 that may be located on a weight-bearing surface, such as a floor 819 of a building. In the illustrated embodiment, the base 802 comprises a generally rectilinear support structure that may be mounted (e.g., bolted) to the floor 819. The support column 801 may be located on and supported by the base 802 and may extend upwards from the top surface of the base 802 in a generally vertical direction. The support column 801 may have a length dimension that extends vertically at least about 2 meters, such as 2-5 meters (e.g., about 3 meters).

In various embodiments discussed in further detail below, the system 100 may enable imaging (e.g., CT scanning) in multiple orientations and along multiple directions. In embodiments, the system 100 may include a first drive mechanism for translating the gantry 40 relative to the support column 801 in a first direction along the direction of arrow 101 in FIG. 1. The first direction 101 may be a generally vertical direction (i.e., perpendicular to the floor 819), which for the purposes of this disclosure may be defined as $\pm 15^\circ$ from true vertical. The system 100 may also include a second drive mechanism for rotating the gantry 40 relative to the support column 801 in the direction indicated by arrow 102. The rotation of the gantry 40 may be with respect to an axis 103 that extends orthogonal to the first direction 101 and may be generally parallel to the floor 819. The axis 103 may extend through the isocenter of the bore 116 of the gantry 40. The system may also include a third drive mechanism for translating the gantry 40 and support column 801 with respect to the base 802 in a second direction indicated by arrow 104 in FIG. 1. The second direction 104 may be a generally horizontal direction (i.e., parallel to the floor 819), which for the purposes of this disclosure may be defined as $\pm 15^\circ$ from true horizontal. The second direction 104 may be orthogonal to both the first direction 101 and to the rotation axis 103.

FIGS. 2A-2C, 3A-3C and 4A-4C illustrate an imaging system 100 in various configurations for performing imaging scans along multiple axes. In FIGS. 2A-2C, the support column 801 may support the gantry 40 in a generally vertical orientation, such that the front and rear faces of the gantry 40 extend parallel to the floor 819 and the imaging axis 114 through the gantry bore 116 extends in a vertical direction (i.e., perpendicular to the floor). The imaging axis 114 of the gantry 40 in this configuration may extend parallel to the length dimension of the vertically-extending support column 801.

The gantry 40 may be displaced along the length of the support column 801 in a generally vertical direction. This is illustrated in FIGS. 2A-2C, which show the gantry 40 displaced vertically from a first position in FIG. 2A with the gantry 40 located proximate a first end of the support column 801 (i.e., opposite the base 802), to a second position in FIG. 2B with the gantry 40 located approximately mid-way along the length of the support column 801, to a third position in FIG. 2C, with the gantry 40 located proximate to a second end of the support column 801 proximate to the base 802. The gantry 40 and the support column 801 may include mating features that confine the displacement of the gantry

40 along the length of the support column 801. As shown in FIGS. 2A-2C, for example, a pair of parallel rails 805, 806 may extend in a vertical direction along the length of the support column 801. A carriage 807 may be mounted to the side of the gantry 40 that attaches to the support column 801. The carriage 807 may include bearing elements (e.g., roller and/or dovetail bearing slides) that engage with the rails 805, 806 to provide linear motion of the carriage 807 and gantry 40 along the length of the support column 801.

A first drive mechanism may drive the displacement of the gantry 40 relative to the support column 801. An example of the first drive system 501 is described below with reference to FIGS. 5A-5D. A controller 810 (see FIG. 4A) may control the operation of the first drive mechanism 501 and thereby control the vertical displacement of the gantry 40. The controller may receive position feedback signals indicative of the position of the gantry 40 along the support column 801, such as from a linear encoder.

The system 100 may also include a patient support 813. The patient support 813 may support a patient 105 in a weight-bearing standing position as shown in FIGS. 2A-2C. The patient support 813 may include a first portion 815 that supports the feet of a patient upon which the patient 105 may stand. A second portion 817 may extend generally perpendicular to the first portion 815 and may provide additional support to the patient 105. For example, the patient 105 may lean against the second portion 817 during a scan and the second portion 817 may help to stabilize the patient 105 and prevent the patient 105 from falling off the patient support 813. In embodiments, the patient support 813 may support the patient 105 in a position that is raised above the floor 819, as shown in FIGS. 2A-2C. The first portion 815 and the second portion 817 may be made of a radiolucent (x-ray transparent) material, such as carbon fiber material.

The system 100 may be used to perform an imaging scan of a patient 105 in a weight-bearing standing position. For example, for an x-ray CT imaging system, the x-ray source and detector may rotate within the gantry 40 around the patient while the gantry 40 is displaced vertically on the support column 801 as shown in FIGS. 2A-2C to perform a helical scan of a patient 105 positioned on the patient support 813. In embodiments, the system 100 may scan over the full length of the patient (e.g., from the top of the patient's cranium to the bottom of the patient's feet) or any selected portion thereof. Following a scan, the gantry 40 may be moved to an out-of-the way position (e.g., to the top of the support column 801 or below the patient's feet) and the patient 105 may be removed from the patient support 813.

The gantry 40 may be attached to the support column 801 such that the gantry 40 may rotate (i.e., tilt) with respect to the support column 801. This is illustrated in FIGS. 3A-3C, which illustrate the gantry 40 tilted from a generally vertical orientation (as shown in FIGS. 2A-2C) with the front and rear faces of the gantry 40 extending parallel to the floor 819 and the imaging axis 114 extending in a vertical direction (i.e., perpendicular to the floor) to a generally horizontal orientation with the front and rear faces of the gantry extending perpendicular to the floor 819 and the imaging axis 114 extending in a horizontal direction (i.e., parallel to the floor). The imaging axis 114 of the gantry 40 in the configuration shown in FIGS. 2A-2C may extend perpendicular to the length dimension of the vertically-extending support column 801.

In embodiments, a rotary bearing may enable the rotation of the gantry 40 with respect to the support column 801. In one embodiment, the rotary bearing may include a first

portion (i.e., bearing race) mounted to the carriage **807** and a second portion (i.e., bearing race) mounted to the gantry **40**. The two bearing portions may rotate concentrically relative to one another such that the gantry **40** may be rotated relative to the carriage **807** and support column **801**. In 5 embodiments, the gantry **40** may rotate at least about 90° relative to the support column **801** (e.g., as is illustrated by FIGS. 2A-2C and FIGS. 3A-3C). In some embodiments, the gantry **40** may rotate at least about 180°, such as at least about 270°, including about 300° or more, relative to the 10 support column **801**.

A second drive mechanism may drive the rotation of the gantry **40** relative to the support column **801**. An example of the second drive system **503** is described below with reference to FIGS. 5A-5D. The system controller **810** (see FIG. 4A) may control the operation of the second drive mechanism **503** and thereby control the rotational angle (tilt) of the gantry **40** relative to the support column **801**. The controller may receive position feedback signals indicative of the rotational position of the gantry **40** with respect to the 20 support column **801**, such as from a rotary encoder.

In some embodiments, the patient support **813** may move from a first configuration as shown in FIGS. 2A-2C to a second configuration as shown in FIGS. 3A-3C. In the configuration of FIGS. 2A-2C, the first portion **815** of the patient support **813** may extend in a generally horizontal direction (i.e., parallel to the floor **819**) and the second portion **817** may extend in a generally vertical direction (i.e., away from the floor **819**). In the configuration of FIGS. 3A-3C, the second portion **817** of the patient support **813** may extend in a generally horizontal direction (i.e., parallel to the floor **819**) and the first portion **815** may extend in a generally vertical direction. Put another way, the patient support **813** may tilt by a predetermined angle (e.g., ~90°) relative to the floor **819** between the configuration shown in FIGS. 2A-2C and the configuration shown in FIGS. 3A-3C. In embodiments, the table configuration of FIGS. 2A-2C may be used for scanning a patient in a weight-bearing standing position and the table configuration of FIGS. 3A-3C may be used for scanning a patient in a lying 30 position, as in conventional x-ray CT systems.

In some embodiments, the patient support **813** may rotate (tilt) with respect to a linkage member **821** to which the patient support **813** is attached. In embodiments, the linkage member **821** may also rotate with respect to the floor **819**. For example, the linkage member **821** may be attached to a base **823** that may be mounted to the floor **819**. The linkage member **821** may rotate relative to the base **823**. The rotation of the linkage member **821** relative to the base **823** may raise and lower the patient support **813** relative to the floor **819**. A table control system may provide coordinated rotational motion of the patient support **813** relative to the linkage member **821** and rotational motion of the linkage member **821** relative to the base **823** to move the table system from the configuration shown in FIGS. 2A-2C to the configuration shown in FIGS. 3A-3C. An example of a patient table system that may be used with the system **100** is described in U.S. patent application Ser. No. 15/685,955 filed on Aug. 24, 2017, the entire contents of which were previously incorporated by reference herein.

FIGS. 3A-3C illustrate the system **100** performing an imaging scan of a patient **105** in a lying position. In particular, for an x-ray CT imaging system, the x-ray source and detector may rotate within the gantry **40** around the patient **105** while the gantry **40** is translated relative to the patient support **813** in a generally horizontal direction to perform a helical scan of a patient **105** lying on the patient

support **813**. In the embodiment shown in FIGS. 3A-3C, the gantry **40** and the support column **801** may translate relative to the patient **105** and patient support **813**, which may be stationary during the scan. The gantry **40** and the support column **801** may translate along the length of the base **802**. As shown in FIGS. 3A-3C, the gantry **40** may be displaced vertically on the support column **801** such that the patient **105** is aligned with the bore **116** of the gantry **40** and the imaging axis **114** extends along the length of the patient **105**. The gantry **40** and the support column **801** may then translate along the base **802** in a horizontal direction from a first position as shown in FIG. 3A with the gantry **40** located over the head of the patient **105**, to a second position as shown in FIG. 3B with the gantry **40** located over the mid-section of the patient **105**, to a third position as shown in FIG. 3C with the gantry **40** located over the feet of the patient **105**. The system **100** may perform a horizontal scan over the full length of the patient **105** or any selected portion thereof.

The base **802** and the support column **801** may include mating features that confine the translation of the support column in a horizontal direction along the length of the base **802**. In the example of FIGS. 3A-3C, the base **802** may include rails or tracks that may mate with corresponding features at the bottom of the support column **801** to guide the translation of the support column **801** in a horizontal direction. A third drive mechanism may drive the translation of the support column **801** relative to the base **802**. An example of a third drive mechanism **601** for translating the gantry **40** and support column **801** is schematically illustrated in FIGS. 6A-6B. The third drive mechanism **601** may comprise, for example, a belt drive, a drive wheel, a lead screw, a ball screw, a pulley, etc. or various combinations therefore. The third drive mechanism **601** may be mechanically coupled to and driven by one or more motors, which may be located in the support column **801** and/or the base **802**. The system controller **810** (see FIG. 4A) may control the operation of the third drive mechanism **601** and thereby control the horizontal translation of the support column **801** and gantry **40**. The controller **810** may receive position feedback signals indicative of the position of the support column **801** relative to the base **802**, such as from a linear encoder.

FIGS. 4A-4C illustrate the system **100** performing an imaging scan of a patient **105** along a tilted axis. The patient **105** may be supported by the patient support **813** at an oblique angle such that an axis **1014** extending lengthwise through the patient **105** is neither parallel or perpendicular to the floor **819**. This may be achieved, for example, by rotating (tilting) the patient support **813** and patient **105** from a standing position (as shown in FIGS. 2A-2C) or rotating (tilting) the patient support **813** and patient **105** upwards from a lying position (as shown in FIGS. 3A-3C). The controller **810** may control the second drive mechanism **502** to rotate (tilt) the gantry **40** with respect to the support column **801** such that the imaging axis **114** through the bore **116** is parallel to, and optionally collinear with, the patient axis **1014**. The system **100** may perform an imaging scan (e.g., a helical x-ray CT scan) of the patient **105** by moving the gantry **40** in the direction of the tilted patient axis **1014** while maintaining a fixed angle between the gantry **40** and axis **1014**. In various embodiments, the controller **810** of the imaging system **100** may provide a coordinated movement of the gantry **40** relative to the support column **801** in a vertical direction with a movement of the gantry **40** and support column **801** relative to the base **802** in a horizontal direction. The controller **810** may include logic configured to determine the relative vertical and horizontal displace-

ment of the gantry 40 needed to move the gantry 40 along the tilted axis 1014. The controller 810 may send control signals to the first drive mechanism 501 and to the third drive mechanism 601 to provide coordinated vertical and horizontal displacement of the gantry 40. Where the angle of the tilted axis 1014 is known or may be determined, the controller 810 may use simple trigonometric relations to determine the vertical and horizontal displacement of the gantry 40. As in the embodiment of FIGS. 4A-4C, for example, where the tilted axis 1014 is at an angle of 60° relative to horizontal, each cm of the scan along the axis 1014 may include a vertical displacement of the gantry 40 relative to the support column 801 of ~0.87 cm (i.e., $\sin 60^\circ$) and a horizontal displacement of the gantry 40 and support column 801 relative to the base 802 of 0.5 cm (i.e., $\cos 60^\circ$). Thus, the imaging system 100 may perform a scan at any tilt axis 1014, and in embodiments may perform scans along complex axes, such as along a multi-angled or curved axis.

FIGS. 4A-4C illustrate the system 100 performing an imaging scan of a patient 105 along a tilted axis 1014. In particular, for an x-ray CT imaging system, the x-ray source and detector may rotate within the gantry 40 around the patient 105 while the gantry 40 is displaced in both vertical and horizontal directions to perform a helical scan of the patient 105 along a tilted axis 1014. The patient may be supported on a patient support 813 that may be tilted such that the second portion 817 of the patient support 813 may extend parallel to the tilted axis 1014. The gantry 40 may be tilted on the support column 801 to align the gantry imaging axis 814 with the tilted axis 1014. The gantry 40 may be moved in both a vertical and horizontal direction from a first position as shown in FIG. 4A with the gantry 40 located over the head of the patient 105, to a second position as shown in FIG. 4B with the gantry 40 located over the mid-section of the patient 105, to a third position as shown in FIG. 4C with the gantry 40 located over the feet of the patient 105. The system 100 may perform scan over the full length of the patient 105 or any selected portion thereof.

FIGS. 5A-5D illustrate an example of a support column 801 for a multi-axis imaging system. FIG. 5A is a front perspective view of a support column 801. FIG. 5B is a rear, partially-transparent perspective view of the support column 801 showing an interior portion thereof. FIG. 5C is a cross-section view taken lengthwise through the support column 801. FIG. 5D illustrates the first and second drive mechanisms 501, 503 with the surrounding support structure of the support column 801 removed.

The support column 801 may be formed of a high-strength structural material, such as aluminum. The support column 801 may include a hollow interior that may form one or more interior housings or compartments. In the embodiment of FIGS. 5A-5C, the support column 801 may include a first interior housing 505 that extends lengthwise in a front portion of the support column 801, and at least one second interior housing 507 in a rear portion of the support column. As shown in FIG. 2A, for example, a front cover 809 may cover the first interior housing 505, and an elongated opening or slot 811 may provide access to the first interior housing 505. The parallel rails 805, 806 which are engaged by the bearing elements 502, 504 of the carriage 807 may be attached to the front face of the support column 801. In some embodiments, the beds on which the rails 805, 806 are mounted may be counter-machined to offset any deflection of the support column 801 that may result from the load of the cantilevered gantry 40 as it travels up and down the column 801.

The first drive mechanism 501 for driving the vertical translation of the gantry 40 may be located on the support column 801. The first drive mechanism 501 may comprise a linear actuator, such as a lead screw or ball screw system. As shown in FIGS. 5A and 5D, a threaded shaft 509 may extend lengthwise within the first interior housing 505 of the support column 801. A motor 511, which may be located in the second interior housing 507 of the support column 801, may be geared into the threaded shaft 509 to drive the rotation of the shaft 509. In one embodiment, the motor 511 may drive a toothed belt 513 that may engage with a sprocket wheel 515 to drive the rotation of the threaded shaft 509. An arm 517 may extend from the carriage 807 into the first interior housing 505 (e.g., through the opening 811 shown in FIG. 2A). A nut 519 on the end of the arm 517 may engage with the threaded shaft 509. The rotation of the threaded shaft 509 may cause the nut 519 to reciprocate up and down along the length of the shaft 509. The reciprocation of the nut 519 on the shaft 509 may drive the vertical displacement of the carriage 807 and gantry 40 with respect to the support column 801. A controller 810 (see FIG. 4A) may control the operation of the first drive mechanism 501 and thereby control the vertical displacement of the gantry 40. The controller may receive position feedback signals indicative of the position of the gantry 40 along the support column 801, such as from a linear encoder.

The first drive mechanism 501 may be non-backdrivable under normal and/or rated operating loads (which could be, for example, up to about 6500 lbs.). This may provide improved safety of the system 100. In embodiments, the first drive mechanism 501 may include a non-backdrivable lead screw. Alternately, the first drive mechanism 501 may be a backdrivable actuator, such as a ball screw. An additional safety mechanism, such as a spring-set brake, may be utilized to prevent backdriving under load.

The second drive mechanism 503 for driving the rotation of the gantry 40 relative to the support column 801 may be located on the carriage 807. In the embodiment of FIGS. 5A-5D, a motor 521 may be attached to one side of the carriage 807. The motor 521 may be geared into a sprocket wheel 523 that is adjacent to the outer race 527 of a rotary bearing 525. The outer race 527 of the bearing 525 may be attached to the gantry 40 and the inner race 529 of the bearing 525 may be attached to the carriage 807. A toothed belt 531 may extend over at least a portion of the outer circumference of the outer race 527 and may engage with a toothed surface of the outer race 527. The belt 531 may be looped over the sprocket wheel 523 that is driven by the motor 521 such that the rotation of the sprocket wheel 523 in a clockwise or counterclockwise direction causes a corresponding rotation of the outer race 527 and gantry 40 relative to the inner race 529, carriage 807 and support column 801. The second drive mechanism 503 preferably includes minimal lash between the belt 531, sprocket wheel 523 and toothed surface of the outer race 527 to enable precise rotational control of the gantry 40. In embodiments, the belt 531 may not be continuous, and opposing ends of the belt 531 may be bolted or clamped to the outer race 537 to minimize slippage and/or backlash. In embodiments, the belt 531 may be clamped to enable at least about 270°, including about 300° or more, of rotation of the gantry 40 relative to the support column 801. In some embodiments, a brake system may be selectively engaged to hold the rotational (tilt) position of the gantry 40 (e.g., during a scan). The controller 810 (see FIG. 10A) may control the operation of the second drive mechanism 503 and thereby control the rotational displacement of the gantry 40. The controller may

receive position feedback signals indicative of the rotational position of the gantry 40 with respect to the support column 801, such as from a rotary encoder.

FIGS. 6A-6B illustrate a base 802 of a multi-axis imaging system 100 according to an embodiment. The base 802 may include a generally rectangular support frame 602. A pair of parallel support rails 603, 605 may extend lengthwise along the base 802. The support rails 603, 605 may support the support column 801 and inhibit deflection as the support column 801 traverses along the length of the base 802. A pair of guide rails 607, 609 may extend along a bottom surface of the base 802 and may be parallel to the support rails 603, 605. A platform 611 may be located over the support rails 603, 605. The support column 801 may be attached (e.g., screwed or bolted) to the upper surface of the platform 611. The platform 611 may include bearing elements (e.g., bearing slides) that engage with the guide rails 607, 609 to provide linear motion of the platform 611, support column 801 and gantry 40 along the length of the base 802.

The third drive mechanism 601 for driving the horizontal translation of the gantry 40 and support column 801 may be located on the base 802. The third drive mechanism 601 may comprise a motor 613 that may be attached to the platform 611. The motor 613 may be geared into a sprocket wheel 615. A drive belt 617 may extend lengthwise along the bottom surface of the base 802. A portion of the drive belt 617 adjacent to the platform 611 may be looped over and engage with the sprocket wheel 615 that is driven by the motor 613. The driving of the sprocket wheel 615 by the motor 613 may cause the sprocket wheel 615 and platform 611 to traverse up and down the length of the drive belt 617, thereby driving the translation of the platform 611, support column 801 and gantry 40 along the length of the base 802. The controller 810 (see FIG. 4A) may control the operation of the third drive mechanism 601 and thereby control the translation of the gantry 40 and support column 801 relative to the base. The controller 810 may receive position feedback signals indicative of the translational position of the gantry 40 and support column 801 on the base 802, such as from a linear encoder.

The base 802 may include a cover 619 to protect the internal components of the base 802. The cover 619 may be made of a flexible material and may be wound on a spool 621 as shown in FIG. 6A. The spool 621 may be enclosed within a housing 623 located at an end of the base 802. One end of the cover 619 may be attached to the platform 611 and/or the support column 801 (e.g., using hooks or similar attachment mechanism). The spool 621 may be spring-loaded to maintain a suitable tension on the cover 619. As the support column 801 translates away from the housing 623, the cover 619 may be extended from the housing 623 by being unwound from the spool 621 and as the support column translates towards the housing 623 the cover 619 may be retracted into the housing 623 by being wound onto the spool 621 (e.g., similar to the operation of a roller shade for windows). The base 802 may include a pair of covers 619 attached to opposite sides of the support column 801, where the covers 619 extend and retract from opposite sides of the base 802 as the support column 801 translates. FIGS. 1-4C illustrate the base with extending/retracting covers 619 attached to the support column 801.

FIGS. 7A-7E illustrate a gantry 40 of a multi-axis imaging system 100 according to an embodiment. FIG. 7A is an exploded view of a gantry 40 that illustrates an outer shell 42 of the gantry, a rotor 41 and a bearing assembly 700. The outer shell 42 may comprise a high-strength structural material, such as aluminum. The outer shell 42 may have an

outer circumferential wall 406 that may extend around the periphery of the gantry 40 to enclose the rotating components of the gantry 40 (e.g., x-ray source, detector, etc.), which may be attached to the rotor 41. The outer shell 42 may also include a side wall 412 that may extend from the outer circumferential wall 406 to a bore 116 of the gantry 40 and may enclose the rotating components around one side of the rotating portion. The side wall 412 may form a first outer face 702 of the gantry 40 and may at least partially define the size of the bore 116 of the gantry. A lip portion 701 may extend from the outer circumferential wall 406 around the interior periphery of the gantry shell 42. The lip portion 701 may provide a mounting surface of the bearing assembly 700, as described further below. The lip portion 701 may be offset from the second outer face 704 of the gantry 40 by a distance sufficient to accommodate at least a portion of the bearing assembly 700 inside the outer circumferential wall 406 of the gantry shell 42.

The outer shell 42 of the gantry 40 is shown in a partial cutaway view through the outer circumferential wall 406 in FIG. 7A. As shown in FIG. 7A, the outer circumferential wall 406 may have a larger cross-section thickness at a proximal end 706 of the gantry 40 where the gantry 40 is attached to the support column 801 than at the distal or unsupported end 708 of the gantry 40. The proximal end 706 of the gantry 40 may include a generally circular-shaped flange portion 710 that may be attached to the outer race 527 of the rotary bearing 525 shown in FIGS. 5A-5D.

One or more openings 712 may be provided through the outer circumferential wall 406 as shown in FIG. 7A. The openings 712 may provide air-flow cooling of the components within the gantry 40. In one embodiment, a first set of one or more openings 712a may be located at the proximal end 706 of the gantry 40 and a second set of one or more openings 712b may be located at the distal end 708 of the gantry 40. One or more fans (not illustrated) may be located adjacent to the second set of opening(s) 712b and may operate to suck ambient air in through the first set of opening(s) 712a, over the components within the gantry 40 and out through opening(s) 712b. Alternately or in addition, one or more fans may be located adjacent to the first set of opening(s) 712a and may blow air through the gantry 40 and out through opening(s) 712b. In further embodiments, the direction of airflow may be reversed, such that air is sucked into the gantry 40 through opening(s) 712b and exits the gantry 40 through opening(s) 712(a).

The bearing assembly 700 according to one embodiment is shown in FIGS. 7A and 7C. FIG. 7A is an exploded view showing the bearing assembly 700 attached to the rotor 41. FIG. 7C illustrates the assembled gantry 40 in a partial cut-away view showing the bearing assembly 700 attached to the rotor 41 and to the gantry shell 42. As shown in FIG. 7C, the bearing assembly 700 includes a first race 703 that is attached to the lip portion 701 of the outer shell 42 of the gantry 40, and a second race 705 that is attached to the rotor 41. A bearing element is provided between the first race 703 and the second race 705, and is configured to allow the second race 705 (along with the rotor 41 to which it is attached) to rotate concentrically within the first race 703, preferably with minimal friction, thereby enabling the rotor 41 to rotate with respect to the outer shell 42 of the gantry 40. In the embodiment of FIGS. 7A and 7C, the second race 705 may be a separate component that is firmly secured around the outer circumference of the rotor 41 (e.g., using mechanical fasteners). Alternately, the second race 705 may be formed as an integral part of the rotor 41.

In various embodiments, the first race 703 of the bearing assembly 700 may be mounted to the outer shell 42 of the gantry 40 using a limited suspension system. The suspension system may be configured to accommodate a limited amount of bending/deflection of the cantilevered gantry 40 between the proximal 706 and distal 708 ends of the gantry 40 while ensuring that the bearing assembly 700 rotates within a plane. The present inventors have discovered that attaching an imaging gantry 40 to a support structure 801 at only one end of the gantry 40 in a cantilevered manner may result in a small amount of deflection or bending of the gantry 40 due to the gravity-induced bending moment of the gantry 40. When the gantry 40 is rotated out-of-line with the vertical support column 801, such as for performing a vertical scan as shown in FIGS. 2A-2C or a scan along a tilted axis as shown in FIGS. 3A-3C, the direction of gantry 40 deflection may include a component that is normal to the scan plane of the imaging components (e.g., x-ray source and detector) rotating within the gantry 40. This downward curve or bend of the gantry and bearing on which the rotating components rotate may introduce a sufficiently large “wobble” effect to these components as they rotate between the proximal 706 and distal 708 ends of the gantry 40 to negatively affect image quality of the scan.

Various embodiments include a limited suspension system between the gantry shell 42 and the bearing assembly 700 to provide a small amount of compliance between these components in the direction of gantry deflection such that the bearing assembly 700 may continue to rotate in a plane when the gantry shell 42 is subject to gravity-induced deflection. In the embodiment of FIGS. 7A-7E, this may be achieved by attaching the bearing assembly 700 to the gantry shell 42 at a limited number of attachment points and allowing the portion of the bearing assembly 700 proximate to the distal end 708 of the gantry 40 to effectively “float” over a limited range with respect to the gantry shell 42. In the embodiment of FIGS. 7A-7E, the lip portion 701 of the gantry shell 42 is attached to the first race 703 of the bearing assembly 700 in four locations around the periphery of the gantry 40. It will be understood that the disclosed embodiment is merely exemplary and various embodiments may include more than or less than four attachment points between the gantry shell 42 and the bearing assembly 700.

In the embodiment of FIGS. 7A-7E, the lip portion 701 of the gantry shell 42 may be fastened to the first race 703 of the bearing assembly 700 in two locations 707a, 707b that are more proximate to the proximal end 706 of the gantry 40 than to the distal end 708 of the gantry 40. The two locations 707a, 707b are visible in FIG. 7C. The two locations 707a, 707b may be located on opposite sides of the gantry 40 and may be equidistant from the proximal end 706 of the gantry 40. The lip portion 701 may be rigidly fastened to the first race 703 at locations 707a, 707b using mechanical fasteners, such as a screw 709 that may pass through an opening 714 in the lip portion 701 and into an opening 716 (e.g., a threaded opening) in first race 703. A pair of washers 711a, 711b may be located between the bottom surface of the lip portion 701 and the top surface of the first race 703 and between the top surface of the lip portion 701 and the head of the screw/bolt 709, respectively. The screw 709 may be tightened against the top surface of the lip portion 701 (via washer 711b) to rigidly and securely attach the lip portion 701 to the first race 703 at locations 707a, 707b, as shown in the cross-section view of FIG. 7D. Washer 711a may provide a small gap between the bottom surface of the lip portion 701 and the top surface of the first race 703, as shown in FIG. 7D.

The bearing assembly 700 may be suspended from the gantry shell 42 at two additional locations 713a, 713b that are more proximate to the distal end 708 of the gantry 40 than to the proximal end 706 of the gantry 40. FIGS. 7A-7C and 7E illustrate the attachment of the lip portion 701 of the gantry shell 42 to the first race 703 of the bearing assembly 700 at location 713a. The lip portion 701 may be attached to the first race 703 at location 713b in the same or similar fashion as shown in FIGS. 7A-7C and 7E. Location 713b may be located on the opposite side of the gantry 40 from location 713a. Locations 713a and 713b may be equidistant from the distal end 708 of the gantry 40. In embodiments, attachment locations 707a and 713a may extend along a secant line 720 of the circular gantry 40. The secant line 720 may be parallel to a midline of the gantry 40 extending from the proximal end 706 to the distal end 708 of the gantry 40. Attachment locations 707b and 713a may extend along a second secant line of the gantry 40, where the second secant line may also be parallel to the midline extending between the proximal 706 and distal ends 708 of the gantry 40. The first and second secant lines may be equidistant from the midline.

FIG. 7B is an exploded view of the components used to attach the lip portion 701 to the first race 703 at location 713a. FIG. 7E is a cross-section view showing the lip portion 701 attached to the first race 703 at location 713a. As shown in FIGS. 7B and 7E, the lip portion 701 and first race 703 may be attached using a mechanical fastener, such as a screw 715, that may be similar or identical to the screw 709 used to fasten the lip portion 701 to the first race 703 at locations 707a, 707b. The screw 709 may pass through a relatively large diameter opening 717 in the lip portion 701 of the gantry shell 42. A metal (e.g., steel) plate 719 having a slot 721 may be attached to the bottom surface of the lip portion 701 using mechanical fasteners (e.g., screws or bolts). The bottom surface of the lip portion 701 may include a recess surrounding the opening 717 to accommodate the plate 719. The slot 721 may be oriented along the direction of gravity-induced deflection of the cantilevered gantry 40. For example, the slot 721 may extend along the secant line 720 of the gantry 40 that intersects attachment locations 707a and 713a.

A bushing 723, which may be a bronze bushing, may be located within the slot 721 of the plate 719. The bushing 723 may be dimensioned slightly smaller than the slot 721 along the length of the slot 721 so that there is some degree of compliance between the bushing 723 and the plate 719 in the direction of gantry deflection. This is illustrated in the cross-section view of FIG. 7E. There may be less compliance between the bushing 723 and the plate 709 along the width of the slot 721. Thus, the bushing 723 may be held tight between the side walls of the slot 721 when the gantry 40 is rotated up into the configuration of FIGS. 3A-3C (e.g., for performing a horizontal scan). A first washer 725, which may be a bronze washer, may be located between the bottom surface of the plate 719 and the top surface of the first race 703, and may surround a central opening 724 through the bushing 723. A second washer 727, which may also be a bronze washer, may be located on the top surface of the plate 719 and may surround the central opening 724 through the bushing 723. A Belleville spring washer 729 may be located above the second washer 727 and may surround the central opening 724 through the bushing 723. A third washer 731, which may be a steel washer, may be located above the Belleville spring washer 729.

The screw 715 may be inserted through the third (e.g., steel) washer 731, the Belleville spring washer 729, the

second (e.g., bronze) washer **727**, the central opening **724** of the bushing **723** and the first (e.g., bronze) washer **725** and into an opening **730** (e.g., a threaded opening) in first race **703**. The screw **715** may be fastened against the top surface of the plate **719** (via washers **731**, **729** and **727**) to attach the plate **719** to the first race **703** at location **713a**, as shown in FIG. 7E. The plate **719** may be sandwiched between the first and second washers **725** and **727**. The spring washer **729** may be pre-loaded to maintain the entire stack in compression. The plate **719** may be separated from the top surface of the first race **703** by a gap **733** defined by the first washer **725**. A second gap **735** may separate the bottom surface of the lip portion **701** from the top surface of the first race **703** as shown in FIG. 7E.

The attachment configuration shown in FIGS. 7B and 7E may provide a secure attachment between the gantry shell **42** and the first race **703** of the bearing assembly **700** while allowing the gantry shell **42** to bend or deflect over the bearing assembly without transferring any bend or curvature in the gantry shell **42** to the bearing assembly **700**. This may be achieved by suspending the bearing assembly **700** from the gantry shell **42** in a limited number of attachment locations that are sufficiently spaced to adequately support the bearing assembly **700** and the rotor **41** as it rotates within the gantry **40**. This contrasts with prior attachment techniques in which the bearing assembly **700** is rigidly secured to the gantry shell **42** at regular intervals (e.g. every 15-30° or so) around the periphery of the gantry **40**. In addition, the gap **735** provided between the lip portion **701** and the first race **703** at the distal-most attachment points **713a**, **713b** may be sufficient to prevent the lip portion **701** from imparting a bending force on the first race **703** at the distal end **708** of the gantry **40**. Thus, bearing assembly **700** may remain flat over the entire gantry **40** even when the gantry shell **42** bends due to gravity.

This is schematically illustrated in FIG. 8, which is a side view of a cantilevered gantry **40** mounted to a support column **801**. It will be understood that FIG. 8 is not necessarily to scale and is intended to provide an exaggerated view of the amount of bending of the gantry **40**. For example, for an x-ray CT system, the amount of gantry deflection between the fixed (proximal) and free (distal) ends of the gantry may be 1-2 mm or less. As shown in FIG. 8, by suspending the bearing assembly **700** for the rotor from the gantry shell **42** at a plurality of spaced-apart locations as described above, the bearing assembly **700** is not influenced by the curvature of the gantry shell **42**. Thus, the bearing assembly **700** and the rotor may rotate in a plane **880**, as illustrated by the dashed line. The plane **880** of rotation of the bearing assembly **700** and rotor may be tilted from a horizontal plane, as shown in FIG. 8. This tilt may be corrected for in the software used to process the image data obtained by the imaging system.

Alternately or in addition, the tilt angle of the plane of rotor rotation may be compensated for by mounting the gantry **40** at an angle with respect to the support column **801**. For example, the carriage **807** to which the gantry **40** is attached may have an angled front surface that compensates for the tilt angle of the rotor so that the scan plane is horizontal.

FIG. 9 illustrates a rotor **41** for an x-ray CT imaging system having a plurality of components mounted thereto. The system may be a multi-axis system **100** as described above. The rotor **41** may rotate within a gantry **40**, and may be mounted within the gantry **40** on a bearing assembly **700** as described above with reference to FIGS. 7A-7E. In particular, the rotor **41** may be mounted to the second race

705 of the bearing assembly **700** shown in FIG. 7C using suitable fasteners, such as bolts or screws.

The rotor **41** shown in FIG. 9 includes an x-ray source **43**, a high-voltage generator **44**, a heat exchanger **430**, an x-ray detector **45**, a power supply **63** (e.g., battery system), a computer **46**, a rotor drive mechanism **47**, and a docking system **35** (e.g., for providing intermittent power/data connection between rotating and non-rotation portions of the system). It will be understood that the components described and illustrated are merely exemplary, and other embodiments may omit one or more of these components and may utilize other additional components. For example, in embodiments, power for the rotating portion **101** may be provided by a slip ring or cable system, so that a power supply **63** on the rotating portion **101** may not be needed. In some embodiments, power and/or data may be continuously transferred between the rotating and non-rotating portions via cable, slip ring or wirelessly, in which case the power supply **63**, computer **46** and/or docking system **35** may not be included. Further, the rotation of the rotor may be provided by a drive system on the non-rotating portion, in which case the rotor drive mechanism **47** on the rotor **41** may not be included. Also, it will be understood that other types of imaging systems, such as MRI systems, may use other suitable components for imaging, as are known in the art.

In embodiments, the x-ray source **43** and detector **45** may be configured to perform a helical x-ray CT scan. The detector **45** may comprise a plurality of x-ray sensitive detector elements arranged in a semicircular arc, with the arc center coinciding with the focal spot of the x-ray source. In some embodiments, the x-ray detector may be a flat panel detector, and the system may be configured to perform real time x-ray fluoroscopic and/or cone beam imaging of an object within the bore of the gantry.

In the embodiment of FIG. 9, during an imaging scan, the rotor **41** rotates within the interior of the gantry, while the imaging components such as the x-ray source **43** and x-ray detector **45** obtain imaging data for an object positioned within the bore **116** of the gantry, as is known, for example, in conventional X-ray CT scanners. The rotor drive mechanism **47** may drive the rotation of the rotor **41** around the interior of the gantry **40**. In embodiments, the rotor drive mechanism **47** may include a drive wheel **901** that engages with a belt **903**. The belt **903** may extend around the gantry **40** on a circular rail **905** that may be fixed to the side wall **412** of the gantry shell **42** (see FIG. 7A). The rotor drive mechanism **47** may be controlled by a system controller that controls the rotation and precise angular position of the rotor **41** with respect to the gantry **40**, preferably using position feedback data, such as from an encoder device.

FIGS. 10A-10K illustrate methods of operating an imaging system **100** to perform an imaging scan of a patient **105** according to various embodiments. The patient **105** may be located on a patient support **813** (e.g., a patient table) as described above. A control system **1001** (e.g., a processor and memory) may be operatively coupled to the patient support **813**, as schematically illustrated in FIG. 10A. The control system **1001** may be located partially or completely within the patient support **813** (e.g., within the linkage member **821**) and/or within one or more separate components, such as a workstation, the imaging system **100** or a mobile cart. The control system **1001** may receive position feedback data (e.g., rotary encoder data) from the patient support **813** and may send control signals to the motor(s) of the patient support **813** to cause the motor(s) to move the patient support **813** into a desired configuration. The con-

figuration of the patient support **813** may be a pre-set configuration (e.g., stored in the memory of the control system **1001**) and/or the configuration may be controllably adjusted by a user using a suitable user input device (e.g., buttons, joystick, pendant controller, computer keyboard and/or mouse, touchscreen display, etc.).

The multi-axis imaging system **100** may also include a control system **810** (e.g., a processor and memory). The control system **810** may be coupled to and control the operation of the first drive mechanism **501**, the second drive mechanism **503** and the third drive mechanism **601** to cause the relative translation and rotation of the gantry **40** with respect to the support column **801** and base **802** as described above. The control system **810** may also receive position feedback signals indicative of the relative positions and orientations of the gantry **40**, support column **801** and base **802**, such as from one or more encoders. The control system **810** may also control the operation of the imaging components within the gantry **40**, and may for example, issue command signal(s) to perform an imaging scan.

The control system **810** may be located within the multi-axis imaging system **100**, such as within the support column **801** and/or within one or more separate components, such as a workstation or a mobile cart. In some embodiments, the control system **810** for the multi-axis imaging system **100** may be co-located with the control system **1001** of the patient support **813**. For example, control systems **810** and **1001** may be implemented as separate processes (e.g., software applications) which run on the same computing device.

The control system **810** for the multi-axis imaging system **100** may be coupled to the control system **1001** for the patient support **813** via a communication link **1003**. The communication link **1003** may enable the control system **1001** for the patient support **813** to transmit data regarding the configuration of the patient support **813** to the control system **810** for the multi-axis imaging system **100**. In some embodiments, the communication link **1003** may be a bi-directional link, and the control system **810** for the multi-axis imaging system **100** may send data to the control system **1001** for the patient support **813** indicating the configuration of the multi-axis imaging system **100**.

In various embodiments, the control systems **810**, **1001** for the multi-axis imaging system **100** and the patient support **813** may communicate over communication link **1003** so that each of these components may always know where the other one is relative to it. This may provide an important safety feature to prevent the imaging system **100** from colliding with the patient support **813** or a patient supported thereon. In some embodiments, the multi-axis imaging system **100** and the patient support **813** may be “electronically geared” such that a movement of one of these components may cause a pre-determined counter-movement of the other component. In one embodiment, the control system **1001** for the patient support **813** may be the “master” controller and the control system **810** for the imaging system **100** may be the “slave” controller. In other words, a movement of the patient support **813** may cause the control system **810** of the imaging system **100** to control the system **100** to make a corresponding counter-move.

FIGS. 10A-10K illustrate various motions of the patient support **813** and multi-axis imaging system **100**. In FIG. 10A, the patient support **813** may be in a position for loading or unloading of a patient. The imaging system **100** may be in a standby or “home” position with the support column **801** and gantry **40** translated away from the patient support **813**. The gantry **40** may be rotated in-line with the support

column **801**. The standby or “home” position of the imaging system **100** may inhibit a collision between the imaging system **100** and the patient or the patient support **813**. The patient support **813** in various embodiments may be lowered to a position as shown in FIG. 10A so that the second portion **817** of the patient support **813**, which can support the patient in a lying position, is at a comfortable height for loading and unloading of the patient. For example, the second portion **817** may be at a height of no more than about 50 cm, such as between 30 and 40 cm from the floor. This may allow a patient to easily climb onto or be lowered down onto the patient support **813**, which may be convenient and safe for both the patient and the medical staff members.

The patient support **813** may then be raised from the lowered position of FIG. 10A to a height suitable for an imaging scan (e.g., such that the patient support **813** may be positioned within the bore of the gantry **40**). FIG. 10B illustrates the patient support **813** raised such that it is aligned with the bore of the gantry **40**. In this configuration, the imaging system **100** is ready to perform a horizontal scan of a patient in a lying position. The patient support **813** may be raised or lowered to a suitable height for performing a scan. FIG. 10C illustrates the patient support **813** raised to a maximum height for performing a scan of a patient supported in a horizontal lying position. The control system **810** of the imaging system **100** may send control signals to the first drive mechanism **501** to cause the gantry **40** to translate vertically on the support column **801** in coordination with the movement of the patient support **813** so that the bore of the gantry **40** remains aligned with the second portion **817** of the patient support **813**. In some embodiments, the control system **810** of the imaging system **100** may also send control signals to the third drive mechanism **601** to cause the support column **801** and gantry **40** to translate along the base **802** to maintain a pre-determined separation between the gantry **40** and the tip end of the second portion **817** of the patient support **813** as the patient support **813** is raised and/or lowered. In some embodiments, gantry **40** may move to maintain the outer face of the gantry **40** separated from the tip end of the of the second portion **817** of the patient support **813**. Alternately, the gantry **40** may move to maintain the tip end of the second portion **817** at least partially inside the bore of the gantry **40**.

When the patient support **813** is moved to a desired configuration, the control system **1001** of the patient support **813** may send a signal to the control system **810** of the imaging system **100** indicating that the system is ready to perform a scan. The control system of the imaging system **100** may send control signals to the third drive mechanism **601** to cause the support column **801** and gantry **40** to translate along the base **802** and over the patient support **813** to perform a scan in a horizontal direction, as shown in FIG. 10D. In some embodiments, the patient support **813** may be prohibited from moving until the scan is complete.

To perform a scan along a tilted axis such as shown in FIGS. 4A-4C, the patient support **813** may be pivoted upwards as shown in FIGS. 10E and 10F. In response to the movement of the patient support **813**, the control system **810** of the imaging system **100** may control the first, second and third drive mechanisms **501**, **503**, **601** to perform a coordinated motion of the gantry **40** as shown in FIGS. 10E and 10F. In particular, the second drive mechanism **503** may rotate the gantry **40** relative to the support column **801** to maintain the bore axis of the gantry **40** aligned with the tilt angle of the patient support **813**. The first and third drive mechanisms **501** and **601** may translate the gantry **40** in both a vertical and horizontal direction to maintain the bore of the

gantry **40** in alignment with the tip end of the patient support **813**. The gantry **40** may maintain a pre-determined separation distance from the tip end of the patient support **813** as it follows the position of the patient support **813**. In some embodiments, gantry **40** may move to maintain the outer face of the gantry **40** separated from the tip end of the of the second portion **817** of the patient support **813**. Alternately, the gantry **40** may move to maintain the tip end of the second portion **817** at least partially inside the bore of the gantry **40**.

When the patient support **813** is moved to a desired tilt angle, the control system **1001** of the patient support **813** may send a signal to the control system **810** of the imaging system **100** indicating that the system is ready to perform a scan. The control system of the imaging system **100** may send control signals to the first and third drive mechanisms **501** and **601** to perform a coordinated vertical and horizontal translation of the gantry **40** and perform a scan along a tilted axis, as shown in FIG. **10G**. In some embodiments, the patient support **813** may be prohibited from moving until the scan is complete.

To perform a scan in a vertical direction such as shown in FIGS. **2A-2C**, the patient support **813** may be pivoted upwards as shown in FIGS. **10H** and **10I**. In response to the movement of the patient support **813**, the control system **810** of the imaging system **100** may control the first, second and third drive mechanisms **501**, **503**, **601** to perform a coordinated motion of the gantry **40** as shown in FIGS. **10H** and **10I**. In particular, the second drive mechanism **503** may rotate the gantry **40** relative to the support column **801** to maintain the bore axis of the gantry **40** aligned with the tilt angle of the patient support **813**. The first and third drive mechanisms **501** and **601** may translate the gantry **40** in both a vertical and horizontal direction to maintain the bore of the gantry **40** in alignment with the tip end of the patient support **813**. The gantry **40** may maintain a pre-determined separation distance from the tip end of the patient support **813** as follows the motion of the patient support **813**. In some embodiments, gantry **40** may move to maintain the outer face of the gantry **40** separated from the tip end of the of the second portion **817** of the patient support **813**. Alternately, the gantry **40** may move to maintain the tip end of the second portion **817** at least partially inside the bore of the gantry **40**.

When the patient support **813** is moved to vertical orientation as shown in FIG. **10J**, the control system **1001** of the patient support **813** may send a signal to the control system **810** of the imaging system **100** indicating that the system is ready to perform a vertical scan. The control system of the imaging system **100** may send control signals to the first drive mechanism **501** to translate the gantry **40** down the length of the patient support **801** to perform a vertical scan of the patient, as shown in FIG. **10J**. In some embodiments, the patient support **813** may be prohibited from moving until the scan is complete.

In some embodiments, the patient support **813** may be moved to any arbitrary angle, and may enable the patient to be supported in Trendelenburg and/or reverse Trendelenburg positions. FIG. **10K** shows the patient support **813** tilted down from a horizontal position to support a patient in a Trendelenburg configuration. The gantry **40** may be tilted on the support column **801** in the opposite direction from the patient support **813**, as shown in FIG. **10K**. This may enable imaging of the patient through a variety of different anatomic planes, including, for example, a generally coronal plane (e.g., within $\sim 30^\circ$ of the coronal plane) through at least a portion of the patient's anatomy. This may be useful, for example, for ENT CT scans of the sinus and/or ears. Also, in brachytherapy, the patient support **813** and gantry **40** may

be tilted to a configuration to enable scanning of the prostate region without needing to scan through the patient's femur.

Further embodiments include a multi-axis imaging system **100** that may be utilized for veterinary medicine. A multi-axis imaging system **100** may be used to perform imaging scans of animals, including large animals (e.g., livestock) and/or equine species, in a weight-bearing standing position. An example of the system **100** is shown in FIGS. **11A-11C**. The system **100** in this embodiment is located on a mobile trailer **1101**. However, it will be understood that the system **100** may be a fixed system located in a veterinary hospital/clinic, or another location such as a farm, ranch or zoo. The system **100** includes an imaging gantry **40** attached to a support column **801** in a cantilevered manner, as described above. The gantry **40** may be rotatable with respect to the support column **801** and may also translate along the length of the support column **801** in a vertical direction. Although not visible in FIGS. **11A-11C**, the system **100** may also include a base **802** that supports the support column **801** and gantry **40**, and the support column **801** and gantry **40** may be translatable with respect to the base **802** in a horizontal direction. The system **100** may further include a support stage **1103**. An animal **1105**, such as a horse as shown in FIGS. **11A-11C**, may be positioned on the top surface **1109** of the support stage **1103**. One or more ramp portions **1107** may enable the animal **1105** to easily climb up and down from the top surface **1109**. A cavity **1111** may be provided in the support stage **1103** for housing the gantry **40**, as shown in FIG. **11A**. The cavity **1111** may have a shape that corresponds with the shape of the gantry **40**. When the gantry **40** is lowered into the cavity **1111**, the outer side wall of the gantry **40** may be flush with the top surface **1109**.

The gantry **40** may be raised up from the cavity **1111** to perform a vertical scan of the legs of the animal **1105** standing on the support stage **1103**, as shown in FIG. **11B**. An actuator system may optionally raise the bottom surface **1113** of the cavity **1111** up even with the top surface **1109** of the support stage **1103** in coordination with the raising of the gantry **40**. This may prevent the animal **1105** from accidentally stepping into the cavity **1111**. Following the scan, the gantry **40** may be lowered back into the cavity **1111**, and the animal **1105** may climb down from the support stage **1103**.

FIG. **11C** illustrates the multi-axis imaging system **100** performing a scan of the neck of a standing animal **1105**. The gantry **40** is raised out of the cavity **1111** and positioned such that the neck of the animal **1105** is located within the bore of the gantry. A control system for the imaging system **100** may control the system to perform a coordinated vertical translation of the gantry **40** along the support column **801** and a horizontal translation of the gantry **40** and support column **801** along the base **802** to scan along the neck of the animal **1105**.

Various examples of diagnostic imaging applications that may be performed on a human or animal patient in a weight-bearing position using an embodiment multi-axis imaging system **100** include, without limitation:

Imaging the bones of a foot. The three-dimensional relationships of the bones in the foot in a flatfoot deformity are difficult to assess with standard radiographs. CT scans demonstrate these relationships but are typically made in a non-weightbearing mode. The use of a weightbearing CT or other imaging apparatus may be useful in imaging the feet in patients with severe flexible pesplanus deformities and to better define the anatomical changes that occur.

Imaging of a limb (e.g. leg). Weight-bearing (CT) bilateral long leg hip to ankle examination and non-weight bearing cross-sectional imaging (CT) of the affected limb may be performed on the hip, knee and ankle, for example, and may be useful for determining variations in angulation and alignment accuracy for diagnosis and/or surgical planning.

Imaging of a spine. Weight bearing scanning (e.g., CT scanning) may be useful for improvements in the accurate diagnosis of degenerative spinal disorders by scanning a patient in the “real life” standing position. By scanning in the standing position, the spinal disc and facet joint compresses, which may enable more specific and precise diagnosis of degenerative spine disorders.

Imaging of a joint (e.g., knee). Weight bearing scanning (e.g., CT scanning) of the knee may enable more specific and precise diagnosis of the patella-femoral kinematics and may also be useful in surgical planning.

Angiography. Weight bearing angiography (e.g., CT angiography) may enable more accurate diagnosis, and may be used, for example, to examine the pulmonary arteries in the lungs to rule out pulmonary embolism, a serious but treatable condition. Weight bearing angiography may also be used to visualize blood flow in the renal arteries (those supplying the kidneys) in patients with high blood pressure and those suspected of having kidney disorders. Narrowing (stenosis) of a renal artery is a cause of high blood pressure (hypertension) in some patients and can be corrected. A special computerized method of viewing the images makes renal CT angiography a very accurate examination. This is also done in prospective kidney donors. Weight bearing angiography may also be used to identify aneurysms in the aorta or in other major blood vessels. Aneurysms are diseased areas of a weakened blood vessel wall that bulges out—like a bulge in a tire. Aneurysms are life-threatening because they can rupture. Weight bearing angiography may also be used to identify dissection in the aorta or its major branches. Dissection means that the layers of the artery wall peel away from each other—like the layers of an onion. Dissection can cause pain and can be life-threatening. Weight bearing angiography may also be used to identify a small aneurysm or arteriovenous malformation inside the brain that can be life-threatening. Weight bearing angiography may also be used to detect atherosclerotic disease that has narrowed the arteries to the legs.

FIG. 12 is a system block diagram of a computing device **1300** useful for performing and implementing the various embodiments described above. The computing device **1300** may perform the functions of a control system **810** for a multi-axis imaging system **100** and/or a control system **1001** for a patient support **813**, for example. While the computing device **1300** is illustrated as a laptop computer, a computing device providing the functional capabilities of the computer device **1300** may be implemented as a workstation computer, an embedded computer, a desktop computer, a server computer or a handheld computer (e.g., tablet, a smartphone, etc.). A typical computing device **1300** may include a processor **1301** coupled to an electronic display **1304**, a speaker **1306** and a memory **1302**, which may be a volatile memory as well as a nonvolatile memory (e.g., a disk drive). When implemented as a laptop computer or desktop computer, the computing device **1300** may also include a floppy disc drive, compact disc (CD) or DVD disc drive coupled to the processor **1301**. The computing device **1300** may include

an antenna **1310**, a multimedia receiver **1312**, a transceiver **1318** and/or communications circuitry coupled to the processor **1301** for sending and receiving electromagnetic radiation, connecting to a wireless data link, and receiving data. Additionally, the computing device **1300** may include network access ports **1324** coupled to the processor **1301** for establishing data connections with a network (e.g., LAN coupled to a service provider network, etc.). A laptop computer or desktop computer **1300** typically also includes a keyboard **1314** and a mouse pad **1316** for receiving user inputs.

The foregoing method descriptions are provided merely as illustrative examples and are not intended to require or imply that the steps of the various embodiments must be performed in the order presented. As will be appreciated by one of skill in the art the order of steps in the foregoing embodiments may be performed in any order. Words such as “thereafter,” “then,” “next,” etc. are not necessarily intended to limit the order of the steps; these words may be used to guide the reader through the description of the methods. Further, any reference to claim elements in the singular, for example, using the articles “a,” “an” or “the” is not to be construed as limiting the element to the singular.

The various illustrative logical blocks, modules, circuits, and algorithm steps described in connection with the embodiments disclosed herein may be implemented as electronic hardware, computer software, or combinations of both. To clearly illustrate this interchangeability of hardware and software, various illustrative components, blocks, modules, circuits, and steps have been described above generally in terms of their functionality. Whether such functionality is implemented as hardware or software depends upon the particular application and design constraints imposed on the overall system. Skilled artisans may implement the described functionality in varying ways for each particular application, but such implementation decisions should not be interpreted as causing a departure from the scope of the present invention.

The hardware used to implement the various illustrative logics, logical blocks, modules, and circuits described in connection with the aspects disclosed herein may be implemented or performed with a general purpose processor, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field programmable gate array (FPGA) or other programmable logic device, discrete gate or transistor logic, discrete hardware components, or any combination thereof designed to perform the functions described herein. A general-purpose processor may be a microprocessor, but, in the alternative, the processor may be any conventional processor, controller, microcontroller, or state machine. A processor may also be implemented as a combination of computing devices, e.g., a combination of a DSP and a microprocessor, a plurality of microprocessors, one or more microprocessors in conjunction with a DSP core, or any other such configuration. Alternatively, some steps or methods may be performed by circuitry that is specific to a given function.

In one or more exemplary aspects, the functions described may be implemented in hardware, software, firmware, or any combination thereof. If implemented in software, the functions may be stored on as one or more instructions or code on a non-transitory computer-readable medium. The steps of a method or algorithm disclosed herein may be embodied in a processor-executable software module executed which may reside on a non-transitory computer-readable medium. Non-transitory computer-readable media includes computer storage media that facilitates transfer of

21

a computer program from one place to another. A storage media may be any available media that may be accessed by a computer. By way of example, and not limitation, such non-transitory computer-readable storage media may comprise RAM, ROM, EEPROM, CD-ROM or other optical disk storage, magnetic disk storage or other magnetic storage devices, or any other medium that may be used to carry or store desired program code in the form of instructions or data structures and that may be accessed by a computer. Disk and disc, as used herein, includes compact disc (CD), laser disc, optical disc, digital versatile disc (DVD), floppy disk, and blu-ray disc where disks usually reproduce data magnetically, while discs reproduce data optically with lasers. Combinations of the above should also be included within the scope of non-transitory computer-readable storage media. Additionally, the operations of a method or algorithm may reside as one or any combination or set of codes and/or instructions on a machine readable medium and/or computer-readable medium, which may be incorporated into a computer program product.

The preceding description of the disclosed aspects is provided to enable any person skilled in the art to make or use the present invention. Various modifications to these aspects will be readily apparent to those skilled in the art, and the generic principles defined herein may be applied to other aspects without departing from the scope of the invention. Thus, the present invention is not intended to be limited to the aspects shown herein but is to be accorded the widest scope consistent with the principles and novel features disclosed herein.

What is claimed is:

1. A multi-axis imaging system, comprising:
 - a patient support including a drive system for moving the patient support between a plurality of positions;
 - an imaging gantry with an imaging axis extending through a bore of the imaging gantry;
 - a support column that supports the imaging gantry on one side of the gantry in a cantilevered manner;
 - a base that supports the imaging gantry and the support column;
 - a plurality of drive mechanisms for moving the gantry in at least three degrees of freedom including:
 - a first drive mechanism that translates the gantry in a vertical direction relative to the support column and the base;
 - a second drive mechanism that rotates the gantry with respect to the support column between a first orientation where the imaging axis of the imaging gantry extends in a vertical direction parallel to the support column and a second orientation where the imaging axis of the gantry extends in a horizontal direction parallel with the base; and
 - a third drive mechanism that translates the support column and the gantry in a horizontal direction along the base;
 - a control system that receives data from the patient support, data indicating a position and a tilt angle of the patient support, and sends control signals to one or more of the plurality of drive mechanisms to cause the gantry to move and position a center of the bore of the gantry axially with the patient support in response to the data received from the control system.
2. The multi-axis imaging system of claim 1, wherein the patient support moves between a horizontal position where a longitudinal axis of the patient support parallel to the base; and

22

a vertical position where the longitudinal axis of the patient support is perpendicular to the base; and the gantry moves with the patient support between the horizontal position and the vertical position, axially aligning the bore of the gantry with the longitudinal axis of the patient support.

3. The multi-axis imaging system of claim 2, wherein the patient support moves to a third position where the patient support is in an angled position, positioning the longitudinal axis of the patient at an angle greater than 0 degrees and less than 90 degrees relative to the base.

4. The multi-axis imaging system of claim 2, wherein the second drive mechanism is configured to rotate the gantry between a first orientation, wherein an imaging axis extending through a bore of the gantry extends in a vertical direction, and a second orientation, wherein an imaging axis extending through the bore of the gantry extends in a horizontal direction.

5. The multi-axis imaging system of claim 1, wherein the first drive mechanism is a non-backdrivable drive mechanism including a motor geared into a lead screw that extends along a length of the support column, and a carriage connected with the gantry has a nut fixed thereto that engages with the lead screw such that a rotation of the lead screw drives a translation of the carriage and the gantry in a vertical direction relative to the support column, the lead screw and the nut are free from backdriving under load.

6. The multi-axis imaging system of claim 5, wherein the support column comprises a plurality of rails extending parallel to one another over a surface of the support column and the gantry is mounted to a carriage having bearing elements that engage with the rails to displace the gantry in a vertical direction relative to the support column.

7. The multi-axis imaging system of claim 5, wherein the first drive mechanism comprises a motor geared into a threaded shaft that extends along the length of the support column, and the carriage has a nut fixed thereto that engages with the threaded shaft such that a rotation of the threaded shaft drives a translation of the carriage and the gantry in a vertical direction relative to the support column.

8. The multi-axis imaging system of claim 7, wherein the second drive mechanism is mounted to the carriage.

9. The multi-axis imaging system of claim 8, wherein the second drive mechanism comprises a motor mechanically coupled to a first race of a rotary bearing such that the motor drives the rotation of the first race relative to a second race of the rotary bearing, and the first race is attached to the gantry and the second race is attached to the carriage.

10. The multi-axis imaging system of claim 9, wherein the motor drives a drive wheel that engages with a drive belt that extends over a surface of the first race and drives the rotation of the first race relative to the second race.

11. The multi-axis imaging system of claim 10, wherein opposing ends of the drive belt are attached to the first race.

12. The multi-axis imaging system of claim 5, wherein the base comprises at least one rail extending along a length of the base, and the support column is mounted to a platform having at least one bearing element that engages with the at least one rail to displace the support column and the gantry in a horizontal direction with respect to the base.

13. The multi-axis imaging system of claim 12, wherein the third drive mechanism comprises a drive belt extending along the length of the base parallel to the at least one rail and a motor mounted to the platform that drives a drive wheel that engages with the drive belt to drive the displacement of the support column and the gantry.

23

14. The multi-axis imaging system of claim 13, wherein the base comprises at least one cover attached to the platform and/or the support column that extends from and retracts into a housing based on the translation of the support column relative to the base.

15. A method of operating a multi-axis imaging system comprising a moveable imaging gantry attached to a support column that supports the imaging gantry on one side of the gantry in a cantilevered manner, a base that supports the imaging gantry and the support column, a first drive mechanism that translates the gantry in a vertical direction relative to the support column and the base, a second drive mechanism that rotates the gantry with respect to the support column; and a third drive mechanism that translates the support column and the gantry in a horizontal direction along the base, the method comprising:

receiving, from a control system of a moveable patient support, data indicating a position and a tilt angle of the patient support; and

sending control signals to one or more drive mechanisms of the multi-axis imaging system to cause the gantry to move in one or more degrees of freedom to maintain a bore of the gantry in a spaced away relationship from the patient support, the bore of the gantry aligned with the patient support in response to the data received from the control system of the moveable patient support;

wherein the gantry is moveable by translating in a first direction and in a second direction and by rotating with

24

respect to an axis extending in a third direction, where the first, second and third directions are mutually orthogonal;

wherein the gantry is axially aligned with the patient support by a distance sufficient to prevent a surface of the gantry from colliding with the patient support or a patient supported thereon while the patient support is moving.

16. The method of claim 15, wherein the second drive mechanism is configured to rotate the gantry between a first orientation, wherein an imaging axis extending through the bore of the gantry extends in a vertical direction, and a second orientation, wherein an imaging axis extending through the bore of the gantry extends in a horizontal direction.

17. The method of claim 16 further comprising: scanning with the gantry in a first position where the patient support is in a horizontal position, positioning a longitudinal axis of the patient support parallel to the base; and

scanning with the gantry in a second position where the patient support is in a vertical position, position the longitudinal axis of the patient support perpendicular to the base.

18. The method of claim 17 further comprising scanning with the gantry in a third position where the patient support is in an angled position, positioning the longitudinal axis of the patient at an angle greater than 0 degrees and less than 90 degrees relative to the base.

* * * * *