



US011892289B2

(12) **United States Patent**
Johansson et al.

(10) **Patent No.:** **US 11,892,289 B2**
(45) **Date of Patent:** ***Feb. 6, 2024**

(54) **MANUAL CALIBRATION OF IMAGING SYSTEM**

(71) Applicant: **PHILIPS IMAGE GUIDED THERAPY CORPORATION**, San Diego, CA (US)

(72) Inventors: **Andreas Johansson**, San Diego, CA (US); **Jason Y. Sproul**, Watertown, MA (US)

(73) Assignee: **PHILIPS IMAGE GUIDED THERAPY CORPORATION**, San Diego, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 110 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **17/194,729**

(22) Filed: **Mar. 8, 2021**

(65) **Prior Publication Data**
US 2021/0190476 A1 Jun. 24, 2021

Related U.S. Application Data

(63) Continuation of application No. 14/107,861, filed on Dec. 16, 2013, now Pat. No. 10,942,022.
(Continued)

(51) **Int. Cl.**
G01B 9/02091 (2022.01)
A61B 5/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **G01B 9/02091** (2013.01); **A61B 5/0066** (2013.01); **A61B 5/0073** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC G01B 9/02091; G01B 9/02089; G01B 9/02072; G01B 21/045; A61B 5/0073;
(Continued)

(56) **References Cited**
U.S. PATENT DOCUMENTS
3,301,258 A 1/1967 Werner
3,617,880 A 11/1971 Cormack et al.
(Continued)

FOREIGN PATENT DOCUMENTS
EP 1041373 A2 10/2000
EP 01172637 A1 1/2002
(Continued)


OTHER PUBLICATIONS

Bell, Malcolm R., et al. "Validation of a new UNIX-based quantitative coronary angiographic system for the measurement of coronary artery lesions." Catheterization and cardiovascular diagnosis 40.1 (1997): 66-74. (Year: 1997).*
(Continued)

Primary Examiner — Vu Le
Assistant Examiner — Tracy Mangialaschi

(57) **ABSTRACT**
The invention generally relates to methods for manually calibrating imaging systems such as optical coherence tomography systems. In certain aspects, an imaging system displays an image showing a target and a reference item. A user looks at the image and indicates a point within the image near the reference item. A processor detects an actual location of the reference item within an area around the indicated point. The processor can use an expected location of the reference item with the detected actual location to calculate a calibration value and provide a calibrated image. In this way, a user can identify the actual location of the reference point and a processing algorithm can give precision to the actual location.

21 Claims, 16 Drawing Sheets

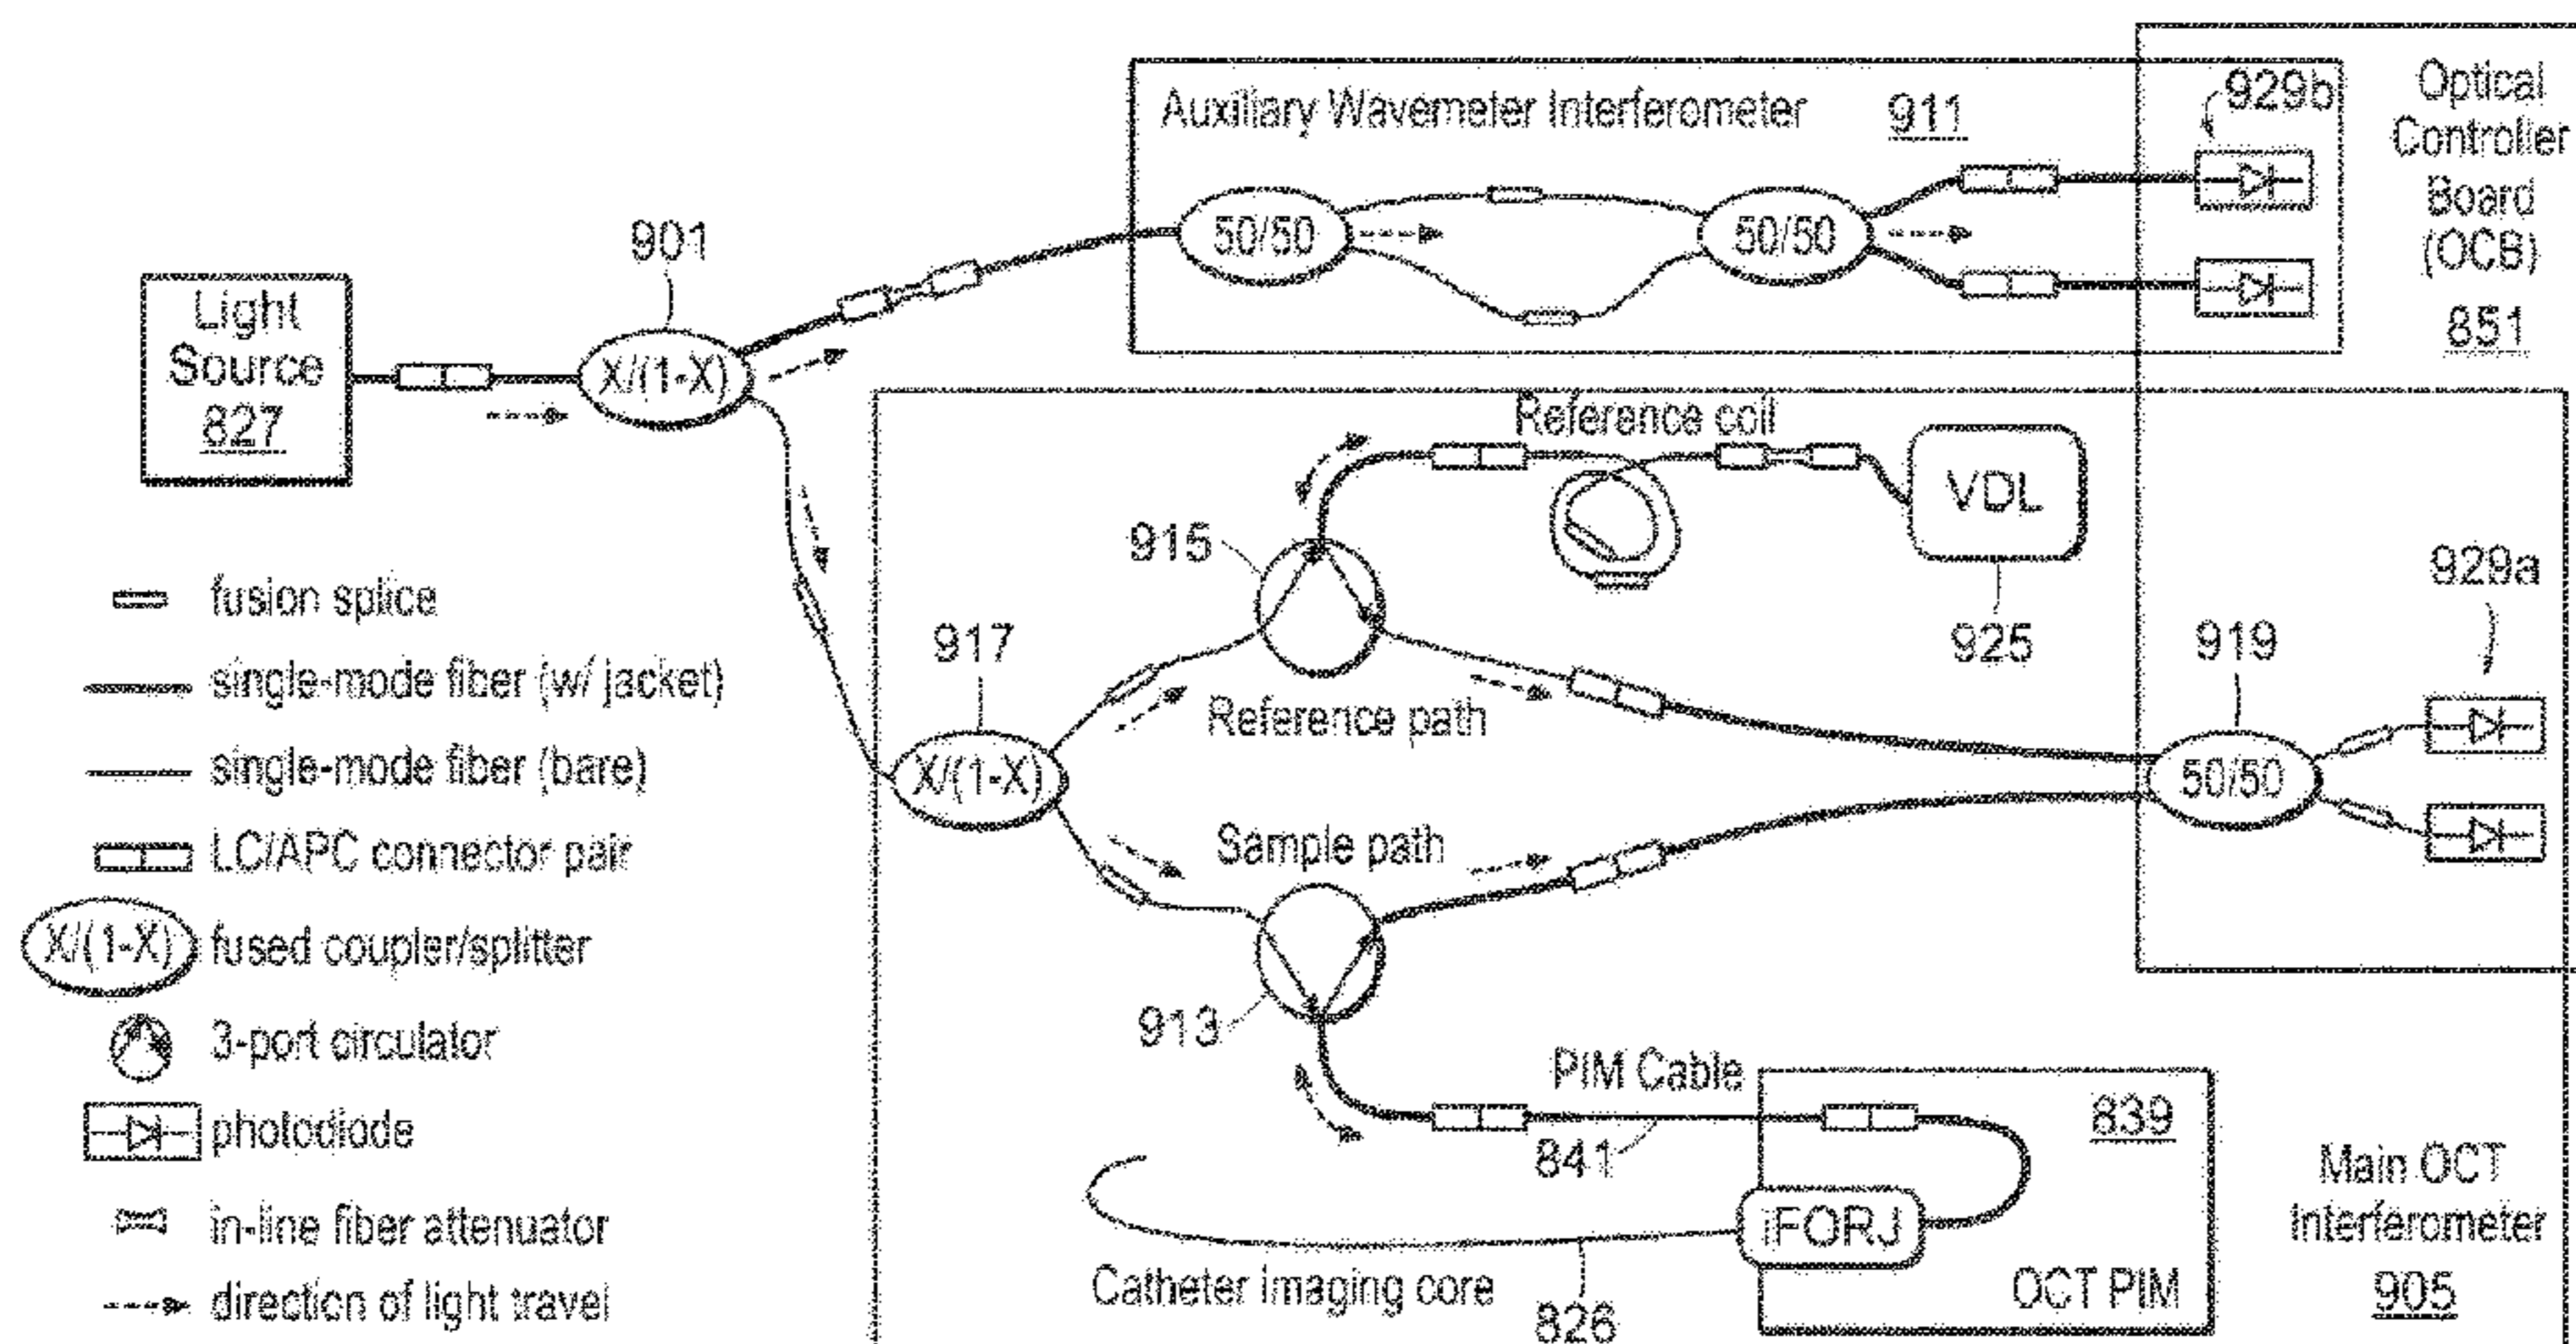

Related U.S. Application Data				
		5,039,193 A	8/1991	Snow et al.
		5,040,548 A	8/1991	Yock
		5,041,108 A	8/1991	Fox et al.
(60)	Provisional application No. 61/739,881, filed on Dec. 20, 2012.	5,054,492 A	10/1991	Scribner et al.
		5,065,010 A	11/1991	Knute
		5,065,769 A	11/1991	de Toledo
(51)	Int. Cl.	5,085,221 A	2/1992	Ingebrigtsen et al.
	<i>G01B 9/02</i> (2022.01)	5,095,911 A	3/1992	Pomeranz
	<i>G01B 21/04</i> (2006.01)	5,100,424 A	3/1992	Jang et al.
	<i>G06T 7/80</i> (2017.01)	5,120,308 A	6/1992	Hess
	<i>G01B 9/02055</i> (2022.01)	5,125,137 A	6/1992	Corl et al.
		5,135,486 A	8/1992	Eberle et al.
(52)	U.S. Cl.	5,135,516 A	8/1992	Sahatjian et al.
	CPC <i>G01B 9/02072</i> (2013.04); <i>G01B 9/02089</i>	5,155,439 A	10/1992	Holmbo et al.
	(2013.01); <i>G01B 21/045</i> (2013.01); <i>G06T 7/80</i>	5,158,548 A	10/1992	Lau et al.
	(2017.01); <i>A61B 5/7475</i> (2013.01); <i>A61B</i>	5,163,445 A	11/1992	Christian et al.
	<i>2560/0223</i> (2013.01); <i>G06T 2207/10101</i>	5,167,233 A	12/1992	Eberle et al.
	(2013.01); <i>G06T 2207/20101</i> (2013.01); <i>G06T</i>	5,174,295 A	12/1992	Christian et al.
	<i>2207/30101</i> (2013.01)	5,176,141 A	1/1993	Bom et al.
		5,176,674 A	1/1993	Hofmann
(58)	Field of Classification Search	5,178,159 A	1/1993	Christian
	CPC A61B 5/0066; A61B 5/7475; A61B	5,183,048 A	2/1993	Eberle
	2560/0223; G06T 7/80; G06T	5,188,632 A	2/1993	Goldenberg
	2207/20101; G06T 2207/30101; G06T	5,201,316 A	4/1993	Pomeranz et al.
	2207/10101	5,202,745 A	4/1993	Sorin et al.
	See application file for complete search history.	5,203,779 A	4/1993	Muller et al.
		5,220,922 A	6/1993	Barany
		5,224,953 A	7/1993	Morgentaler
		5,226,421 A	7/1993	Frisbie et al.
(56)	References Cited	5,240,003 A	8/1993	Lancee et al.
	U.S. PATENT DOCUMENTS	5,240,437 A	8/1993	Christian
		5,242,460 A	9/1993	Klein et al.
		5,243,988 A	9/1993	Sieben et al.
		5,257,974 A	11/1993	Cox
	3,789,841 A 2/1974 Antoshkiw	5,266,302 A	11/1993	Peyman et al.
	3,841,308 A 10/1974 Tate	5,267,954 A	12/1993	Nita
	4,140,364 A 2/1979 Yamashita et al.	5,301,001 A	4/1994	Murphy et al.
	4,274,423 A 6/1981 Mizuno et al.	5,312,425 A	5/1994	Evans et al.
	4,344,438 A 8/1982 Schultz	5,313,949 A	5/1994	Yock
	4,398,791 A 8/1983 Dorsey	5,313,957 A	5/1994	Little
	4,432,370 A 2/1984 Hughes et al.	5,319,492 A	6/1994	Dorn et al.
	4,552,554 A 11/1985 Gould et al.	5,321,501 A	6/1994	Swanson et al.
	4,577,543 A 3/1986 Wilson	5,325,198 A	6/1994	Hartley et al.
	4,676,980 A 6/1987 Segal et al.	5,336,178 A	8/1994	Kaplan et al.
	4,682,895 A 7/1987 Costello	5,346,689 A	9/1994	Peyman et al.
	4,733,665 A 3/1988 Palmaz	5,348,017 A	9/1994	Thornton et al.
	4,744,619 A 5/1988 Cameron	5,348,481 A	9/1994	Ortiz
	4,762,129 A 8/1988 Bonzel	5,353,798 A	10/1994	Sieben
	4,766,386 A 8/1988 Oliver et al.	5,358,409 A	10/1994	Obara
	4,771,774 A 9/1988 Simpson et al.	5,358,478 A	10/1994	Thompson et al.
	4,794,931 A 1/1989 Yock	5,368,037 A	11/1994	Eberle et al.
	4,800,886 A 1/1989 Nestor	5,373,845 A	12/1994	Gardineer et al.
	4,803,639 A 2/1989 Steele et al.	5,373,849 A	12/1994	Maroney et al.
	4,816,567 A 3/1989 Cabilly et al.	5,375,602 A	12/1994	Lancee et al.
	4,819,740 A 4/1989 Warrington	5,377,682 A	1/1995	Ueno et al.
	4,821,731 A 4/1989 Martinelli et al.	5,383,853 A	1/1995	Jung et al.
	4,824,435 A 4/1989 Giesy et al.	5,387,193 A	2/1995	Miraki
	4,830,023 A 5/1989 de Toledo et al.	5,396,328 A	3/1995	Jestel et al.
	4,834,093 A 5/1989 Littleford et al.	5,397,355 A	3/1995	Marin et al.
	4,841,977 A 6/1989 Griffith et al.	5,405,377 A	4/1995	Cragg
	4,864,578 A 9/1989 Proffitt et al.	5,411,016 A	5/1995	Kume et al.
	4,873,690 A 10/1989 Adams	5,419,777 A	5/1995	Hofling
	4,877,314 A 10/1989 Kanamori	5,421,338 A	6/1995	Crowley et al.
	4,887,606 A 12/1989 Yock et al.	5,423,806 A	6/1995	Dale et al.
	4,917,085 A 4/1990 Smith	5,427,118 A	6/1995	Nita et al.
	4,917,097 A 4/1990 Proudian	5,431,673 A	7/1995	Summers et al.
	4,928,693 A 5/1990 Goodin et al.	5,436,759 A	7/1995	Dijaili et al.
	4,932,413 A 6/1990 Shockey et al.	5,439,139 A	8/1995	Brovelli
	4,932,419 A 6/1990 de Toledo	5,443,457 A	8/1995	Ginn et al.
	4,948,229 A 8/1990 Soref	5,453,575 A	9/1995	O'Donnell et al.
	4,951,677 A 8/1990 Crowley et al.	5,456,693 A	10/1995	Conston et al.
	4,969,742 A 11/1990 Falk et al.	5,459,570 A	10/1995	Swanson et al.
	4,987,412 A 1/1991 Vaitekunas et al.	5,480,388 A	1/1996	Zadini et al.
	4,993,412 A 2/1991 Murphy-Chutorian	5,485,845 A	1/1996	Verdonk et al.
	4,998,972 A 3/1991 Chin et al.	5,492,125 A	2/1996	Kim et al.
	5,000,185 A 3/1991 Yock	5,496,997 A	3/1996	Pope
	5,024,234 A 6/1991 Leary et al.	5,507,761 A	4/1996	Duer
	5,025,445 A 6/1991 Anderson et al.	5,512,044 A	4/1996	Duer
	5,032,123 A 7/1991 Katz et al.	5,514,128 A	5/1996	Hillsman et al.
	5,037,169 A 8/1991 Chun			

(56)

References Cited

U.S. PATENT DOCUMENTS

5,529,674 A	6/1996	Hedgcoth	6,148,095 A	11/2000	Prause et al.
5,541,730 A	7/1996	Chaney	6,151,433 A	11/2000	Dower et al.
5,546,717 A	8/1996	Penczak et al.	6,152,877 A	11/2000	Masters
5,546,948 A	8/1996	Hamm et al.	6,152,878 A	11/2000	Nachtomy et al.
5,565,332 A	10/1996	Hoogenboom et al.	6,159,225 A	12/2000	Makower
5,573,520 A	11/1996	Schwartz et al.	6,165,127 A	12/2000	Crowley
5,581,638 A	12/1996	Givens et al.	6,176,842 B1	1/2001	Tachibana et al.
5,586,054 A	12/1996	Jensen et al.	6,179,809 B1	1/2001	Khairkhahan et al.
5,592,939 A	1/1997	Martinelli	6,186,949 B1	2/2001	Hatfield et al.
5,596,079 A	1/1997	Smith et al.	6,190,353 B1	2/2001	Makower et al.
5,598,844 A	2/1997	Diaz et al.	6,200,266 B1	3/2001	Shokrollahi et al.
5,609,606 A	3/1997	O'Boyle	6,200,268 B1	3/2001	Vince et al.
5,630,806 A	5/1997	Inagaki et al.	6,203,537 B1	3/2001	Adrian
5,651,366 A	7/1997	Liang et al.	6,208,415 B1	3/2001	De Boer et al.
5,660,180 A	8/1997	Malinowski et al.	6,210,332 B1	4/2001	Chiao et al.
5,667,499 A	9/1997	Welch et al.	6,210,339 B1	4/2001	Kiepen et al.
5,667,521 A	9/1997	Keown	6,212,308 B1	4/2001	Donald
5,672,877 A	9/1997	Liebig et al.	6,231,518 B1	5/2001	Grabek et al.
5,674,232 A	10/1997	Halliburton	6,245,066 B1	6/2001	Morgan et al.
5,693,015 A	12/1997	Walker et al.	6,249,076 B1	6/2001	Madden et al.
5,713,848 A	2/1998	Dubrul et al.	6,254,543 B1	7/2001	Grunwald et al.
5,745,634 A	4/1998	Garrett et al.	6,256,090 B1	7/2001	Chen et al.
5,771,895 A	6/1998	Slager	6,258,052 B1	7/2001	Milo
5,779,731 A	7/1998	Leavitt	6,261,246 B1	7/2001	Pantages et al.
5,780,958 A	7/1998	Strugach et al.	6,275,628 B1	8/2001	Jones et al.
5,798,521 A	8/1998	Froggatt	6,283,921 B1	9/2001	Nix et al.
5,800,450 A	9/1998	Lary et al.	6,283,951 B1	9/2001	Flaherty et al.
5,803,083 A	9/1998	Buck et al.	6,295,308 B1	9/2001	Zah
5,814,061 A	9/1998	Osborne et al.	6,299,622 B1	10/2001	Snow et al.
5,817,025 A	10/1998	Alekseev et al.	6,312,384 B1	11/2001	Chiao
5,820,594 A	10/1998	Fontirroche et al.	6,325,797 B1	12/2001	Stewart et al.
5,824,520 A	10/1998	Mulligan-Kehoe	6,328,696 B1	12/2001	Fraser
5,827,313 A	10/1998	Ream	6,343,168 B1	1/2002	Murphy et al.
5,830,222 A	11/1998	Makower	6,343,178 B1	1/2002	Burns et al.
5,848,121 A	12/1998	Gupta et al.	6,350,240 B1	2/2002	Song et al.
5,851,464 A	12/1998	Davila et al.	6,364,841 B1	4/2002	White et al.
5,857,974 A	1/1999	Eberle et al.	6,366,722 B1	4/2002	Murphy et al.
5,872,829 A	2/1999	Wischmann et al.	6,367,984 B1	4/2002	Stephenson et al.
5,873,835 A	2/1999	Hastings et al.	6,373,970 B1	4/2002	Dong et al.
5,882,722 A	3/1999	Kydd	6,375,615 B1	4/2002	Flaherty et al.
5,912,764 A	6/1999	Togino	6,375,618 B1	4/2002	Chiao et al.
5,916,194 A	6/1999	Jacobsen et al.	6,375,628 B1	4/2002	Zadno-Azizi et al.
5,921,931 A	7/1999	O'Donnell et al.	6,376,830 B1	4/2002	Froggatt et al.
5,925,055 A	7/1999	Adrian et al.	6,379,352 B1	4/2002	Reynolds et al.
5,949,929 A	9/1999	Hamm	6,381,350 B1	4/2002	Klingensmith et al.
5,951,586 A	9/1999	Berg et al.	6,387,124 B1	5/2002	Buscemi et al.
5,974,521 A	10/1999	Akerib	6,396,976 B1	5/2002	Little et al.
5,976,120 A	11/1999	Chow et al.	6,398,792 B1	6/2002	O'Connor
5,978,391 A	11/1999	Das et al.	6,417,948 B1	7/2002	Chowdhury et al.
5,997,523 A	12/1999	Jang	6,419,644 B1	7/2002	White et al.
6,021,240 A	2/2000	Murphy et al.	6,421,164 B2	7/2002	Tearney et al.
6,022,319 A	2/2000	Willard et al.	6,423,012 B1	7/2002	Kato et al.
6,031,071 A	2/2000	Mandeville et al.	6,426,796 B1	7/2002	Pulliam et al.
6,036,889 A	3/2000	Kydd	6,428,041 B1	8/2002	Wohllebe et al.
6,043,883 A	3/2000	Leckel et al.	6,428,498 B2	8/2002	Uflacker
6,050,949 A	4/2000	White et al.	6,429,421 B1	8/2002	Meller et al.
6,059,738 A	5/2000	Stoltze et al.	6,440,077 B1	8/2002	Jung et al.
6,068,638 A	5/2000	Makower	6,443,903 B1	9/2002	White et al.
6,074,362 A	6/2000	Jang et al.	6,450,964 B1	9/2002	Webler
6,078,831 A	6/2000	Belef et al.	6,457,365 B1	10/2002	Stephens et al.
6,080,109 A	6/2000	Baker et al.	6,459,844 B1	10/2002	Pan
6,091,496 A	7/2000	Hill	6,468,290 B1	10/2002	Weldon et al.
6,094,591 A	7/2000	Foltz et al.	6,475,149 B1	11/2002	Sumanaweera
6,095,976 A	8/2000	Nachtomy et al.	6,480,285 B1	11/2002	Hill
6,097,755 A	8/2000	Guenther, Jr. et al.	6,491,631 B2	12/2002	Chiao et al.
6,099,471 A	8/2000	Torp et al.	6,491,636 B2	12/2002	Chenal et al.
6,099,549 A	8/2000	Bosma et al.	6,501,551 B1	12/2002	Tearney et al.
6,102,938 A	8/2000	Evans et al.	6,504,286 B1	1/2003	Porat et al.
6,106,476 A	8/2000	Cori et al.	6,508,824 B1	1/2003	Flaherty et al.
6,120,445 A	9/2000	Grunwald	6,514,237 B1	2/2003	Maseda
6,123,673 A	9/2000	Eberle et al.	6,520,269 B2	2/2003	Geiger et al.
6,134,003 A	10/2000	Tearney et al.	6,520,677 B2	2/2003	Iizuka
6,139,510 A	10/2000	Palermo	6,535,764 B2	3/2003	Imran et al.
6,141,089 A	10/2000	Thoma et al.	6,538,778 B1	3/2003	Leckel et al.
6,146,328 A	11/2000	Chiao et al.	6,544,217 B1	4/2003	Gulachenski
			6,544,230 B1	4/2003	Flaherty et al.
			6,545,760 B1	4/2003	Froggatt et al.
			6,546,272 B1	4/2003	MacKinnon et al.
			6,551,250 B2	4/2003	Khalil

(56)

References Cited

U.S. PATENT DOCUMENTS

6,566,648 B1	5/2003	Froggatt	6,954,737 B2	10/2005	Kalantar et al.
6,570,894 B2	5/2003	Anderson	6,958,042 B2	10/2005	Honda
6,572,555 B2	6/2003	White et al.	6,961,123 B1	11/2005	Wang et al.
6,579,311 B1	6/2003	Makower	6,966,891 B2	11/2005	Ookubo et al.
6,584,335 B1	6/2003	Haar et al.	6,969,293 B2	11/2005	Thai
6,592,612 B1	7/2003	Samson et al.	6,969,395 B2	11/2005	Eskuri
6,594,448 B2	7/2003	Herman et al.	6,985,234 B2	1/2006	Anderson
6,602,241 B2	8/2003	Makower et al.	7,004,963 B2	2/2006	Wang et al.
6,611,322 B1	8/2003	Nakayama et al.	7,006,231 B2	2/2006	Ostrovsky et al.
6,611,720 B2	8/2003	Hata et al.	7,010,458 B2	3/2006	Wilt
6,612,992 B1	9/2003	Hossack et al.	7,024,025 B2	4/2006	Sathyanarayana
6,615,062 B2	9/2003	Ryan et al.	7,027,211 B1	4/2006	Ruffa
6,615,072 B1	9/2003	Izatt et al.	7,027,743 B1	4/2006	Tucker et al.
6,621,562 B2	9/2003	Durston	7,033,347 B2	4/2006	Appling
6,631,284 B2	10/2003	Nutt et al.	7,035,484 B2	4/2006	Silberberg et al.
6,638,227 B2	10/2003	Bae	7,037,269 B2	5/2006	Nix et al.
6,645,152 B1	11/2003	Jung et al.	7,042,573 B2	5/2006	Froggatt
6,646,745 B2	11/2003	Verma et al.	7,044,915 B2	5/2006	White et al.
6,655,386 B1	12/2003	Makower et al.	7,044,964 B2	5/2006	Jang et al.
6,659,957 B1	12/2003	Vardi et al.	7,048,711 B2	5/2006	Rosenman et al.
6,660,024 B1	12/2003	Flaherty et al.	7,049,306 B2	5/2006	Konradi et al.
6,663,565 B2	12/2003	Kawagishi et al.	7,058,239 B2	6/2006	Singh et al.
6,665,456 B2	12/2003	Dave et al.	7,060,033 B2	6/2006	White et al.
6,669,716 B1	12/2003	Gilson et al.	7,060,421 B2	6/2006	Naundorf et al.
6,671,055 B1	12/2003	Wavering et al.	7,063,679 B2	6/2006	Maguire et al.
6,673,015 B1	1/2004	Glover et al.	7,068,852 B2	6/2006	Braica
6,673,064 B1	1/2004	Rentrop	7,074,188 B2	7/2006	Nair et al.
6,685,648 B2	2/2004	Flaherty et al.	7,095,493 B2	8/2006	Harres
6,689,056 B1	2/2004	Kilcoyne et al.	7,110,119 B2	9/2006	Maestle
6,689,144 B2	2/2004	Gerberding	7,113,875 B2	9/2006	Terashima et al.
6,696,173 B1	2/2004	Naundorf et al.	7,123,777 B2	10/2006	Rondinelli et al.
6,701,044 B2	3/2004	Arbore et al.	7,130,054 B2	10/2006	Ostrovsky et al.
6,701,176 B1	3/2004	Halperin et al.	7,139,440 B2	11/2006	Rondinelli et al.
6,709,444 B1	3/2004	Makower	7,153,299 B1	12/2006	Tu et al.
6,712,836 B1	3/2004	Berg et al.	7,171,078 B2	1/2007	Sasaki et al.
6,714,703 B2	3/2004	Lee et al.	7,175,597 B2	2/2007	Vince et al.
6,719,717 B1	4/2004	Johnson et al.	7,177,491 B2	2/2007	Dave et al.
6,725,073 B1	4/2004	Motamedi et al.	7,190,464 B2	3/2007	Alphonse
6,726,677 B1	4/2004	Flaherty et al.	7,215,802 B2	5/2007	Klingensmith et al.
6,730,107 B2	5/2004	Kelley et al.	7,218,811 B2	5/2007	Shigenaga et al.
6,733,474 B2	5/2004	Kusleika	7,236,812 B1	6/2007	Ballerstadt et al.
6,738,144 B1	5/2004	Dogariu	7,245,125 B2	7/2007	Harer et al.
6,740,113 B2	5/2004	Vrba	7,245,789 B2	7/2007	Bates et al.
6,746,464 B1	6/2004	Makower	7,249,357 B2	7/2007	Landman et al.
6,780,157 B2	8/2004	Stephens et al.	7,291,146 B2	11/2007	Steinke et al.
6,795,188 B2	9/2004	Ruck et al.	7,292,715 B2	11/2007	Furnish
6,795,196 B2	9/2004	Funakawa	7,292,885 B2	11/2007	Scott et al.
6,798,522 B2	9/2004	Stolte et al.	7,294,124 B2	11/2007	Eidenschink
6,822,798 B2	11/2004	Wu et al.	7,300,460 B2	11/2007	Levine et al.
6,830,559 B2	12/2004	Schock	7,335,161 B2	2/2008	Von Arx et al.
6,832,024 B2	12/2004	Gerstenberger et al.	7,337,079 B2	2/2008	Park et al.
6,842,639 B1	1/2005	Winston et al.	7,355,716 B2	4/2008	de Boer et al.
6,847,449 B2	1/2005	Bashkansky et al.	7,356,367 B2	4/2008	Liang et al.
6,855,115 B2	2/2005	Fonseca et al.	7,358,921 B2	4/2008	Snyder et al.
6,856,138 B2	2/2005	Bohley	7,359,062 B2	4/2008	Chen et al.
6,856,400 B1	2/2005	Froggatt	7,359,554 B2	4/2008	Klingensmith et al.
6,856,472 B2	2/2005	Herman et al.	7,363,927 B2	4/2008	Ravikumar
6,860,867 B2	3/2005	Seward et al.	7,366,376 B2	4/2008	Shishkov et al.
6,866,670 B2	3/2005	Rabiner et al.	7,382,949 B2	6/2008	Bouma et al.
6,878,113 B2	4/2005	Miwa et al.	7,387,636 B2	6/2008	Cohn et al.
6,886,411 B2	5/2005	Kjellman et al.	7,391,520 B2	6/2008	Zhou et al.
6,891,984 B2	5/2005	Petersen et al.	7,397,935 B2	7/2008	Kimmel et al.
6,895,106 B2	5/2005	Wang et al.	7,399,095 B2	7/2008	Rondinelli
6,898,337 B2	5/2005	Averett et al.	7,408,648 B2	8/2008	Kleen et al.
6,900,897 B2	5/2005	Froggatt	7,414,779 B2	8/2008	Huber et al.
6,912,051 B2	6/2005	Jensen	7,440,087 B2	10/2008	Froggatt et al.
6,916,329 B1	7/2005	Zhao	7,447,388 B2	11/2008	Bates et al.
6,922,498 B2	7/2005	Shah	7,449,821 B2	11/2008	Dausch
6,937,346 B2	8/2005	Nebendahl et al.	7,450,165 B2	11/2008	Ahiska
6,937,696 B1	8/2005	Mostafavi	RE40,608 E	12/2008	Glover et al.
6,943,939 B1	9/2005	DiJaili et al.	7,458,967 B2	12/2008	Appling et al.
6,947,147 B2	9/2005	Motamedi et al.	7,463,362 B2	12/2008	Lasker et al.
6,947,787 B2	9/2005	Webler	7,463,759 B2	12/2008	Klingensmith et al.
6,949,094 B2	9/2005	Yaron	7,491,226 B2	2/2009	Palmaz et al.
6,952,603 B2	10/2005	Gerber et al.	7,515,276 B2	4/2009	Froggatt et al.
			7,527,594 B2	5/2009	Vardi et al.
			7,534,251 B2	5/2009	WasDyke
			7,535,797 B2	5/2009	Peng et al.
			7,547,304 B2	6/2009	Johnson

(56)

References Cited

U.S. PATENT DOCUMENTS

7,564,949 B2	7/2009	Sattler et al.	8,070,800 B2	12/2011	Lock et al.
7,577,471 B2	8/2009	Camus et al.	8,080,800 B2	12/2011	Hocor et al.
7,583,857 B2	9/2009	Xu et al.	8,088,102 B2	1/2012	Adams et al.
7,603,165 B2	10/2009	Townsend et al.	8,100,838 B2	1/2012	Wright et al.
7,612,773 B2	11/2009	Magnin et al.	8,104,479 B2	1/2012	Glynn et al.
7,633,627 B2	12/2009	Choma et al.	8,108,030 B2	1/2012	Castella et al.
7,645,229 B2	1/2010	Armstrong	8,114,102 B2	2/2012	Galdonik et al.
7,658,715 B2	2/2010	Park et al.	8,116,605 B2	2/2012	Petersen et al.
7,660,452 B2	2/2010	Zwirn et al.	8,125,648 B2	2/2012	Milner et al.
7,660,492 B2	2/2010	Bates et al.	8,126,239 B2	2/2012	Sun et al.
7,666,204 B2	2/2010	Thornton et al.	8,133,199 B2	3/2012	Weber et al.
7,672,790 B2	3/2010	McGraw et al.	8,133,269 B2	3/2012	Flehsenhar et al.
7,680,247 B2	3/2010	Atzinger et al.	8,140,708 B2	3/2012	Zaharia et al.
7,684,991 B2	3/2010	Stohr et al.	8,148,877 B2	4/2012	Jiang et al.
7,711,413 B2	5/2010	Feldman et al.	8,167,932 B2	5/2012	Bourang et al.
7,720,322 B2	5/2010	Prisco	8,172,757 B2	5/2012	Jaffe et al.
7,728,986 B2	6/2010	Lasker et al.	8,177,809 B2	5/2012	Mavani et al.
7,734,009 B2	6/2010	Brunner et al.	8,187,191 B2	5/2012	Hancock et al.
7,736,317 B2	6/2010	Stephens et al.	8,187,267 B2	5/2012	Pappone et al.
7,742,795 B2	6/2010	Stone et al.	8,187,830 B2	5/2012	Hu et al.
7,743,189 B2	6/2010	Brown et al.	8,199,218 B2	6/2012	Lee et al.
7,762,954 B2	7/2010	Nix et al.	8,206,429 B2	6/2012	Gregorich et al.
7,766,896 B2	8/2010	Komkven Volk et al.	8,208,995 B2	6/2012	Tearney et al.
7,773,792 B2	8/2010	Kimmel et al.	8,222,906 B2	7/2012	Wyar et al.
7,775,981 B1	8/2010	Guracar et al.	8,233,681 B2	7/2012	Aylward et al.
7,777,399 B2	8/2010	Eidenschink et al.	8,233,718 B2	7/2012	Klingensmith et al.
7,781,724 B2	8/2010	Childers et al.	8,238,624 B2	8/2012	Doi et al.
7,783,337 B2	8/2010	Feldman et al.	8,239,938 B2	8/2012	Simeral et al.
7,787,127 B2	8/2010	Galle et al.	8,277,386 B2	10/2012	Ahmed et al.
7,792,342 B2	9/2010	Barbu et al.	8,280,470 B2	10/2012	Milner et al.
7,801,343 B2	9/2010	Unal et al.	8,289,284 B2	10/2012	Glynn et al.
7,801,590 B2	9/2010	Feldman et al.	8,289,522 B2	10/2012	Tearney et al.
7,813,609 B2	10/2010	Petersen et al.	8,298,147 B2	10/2012	Huennekens et al.
7,831,081 B2	11/2010	Li	8,298,149 B2	10/2012	Hastings et al.
7,846,101 B2	12/2010	Eberle et al.	8,301,000 B2	10/2012	Sillard et al.
7,853,104 B2	12/2010	Oota et al.	8,309,428 B2	11/2012	Lemmerhirt et al.
7,853,316 B2	12/2010	Milner et al.	8,317,713 B2	11/2012	Davies et al.
7,860,555 B2	12/2010	Saadat	8,323,201 B2	12/2012	Towfiq et al.
7,862,508 B2	1/2011	Davies et al.	8,329,053 B2	12/2012	Martin et al.
7,872,759 B2	1/2011	Tearney et al.	8,336,643 B2	12/2012	Harleman
7,880,868 B2	2/2011	Aoki	8,349,000 B2	1/2013	Schreck
7,881,763 B2	2/2011	Brauker et al.	8,353,945 B2	1/2013	Andreas et al.
7,909,844 B2	3/2011	Alkhatib et al.	8,353,954 B2	1/2013	Cai et al.
7,921,854 B2	4/2011	Hennings et al.	8,357,981 B2	1/2013	Martin et al.
7,927,784 B2	4/2011	Simpson	8,361,097 B2	1/2013	Patel et al.
7,929,148 B2	4/2011	Kemp	8,386,560 B2	2/2013	Ma et al.
7,930,014 B2	4/2011	Huennekens et al.	8,398,591 B2	3/2013	Mas et al.
7,930,104 B2	4/2011	Baker et al.	8,412,312 B2	4/2013	Judell et al.
7,936,462 B2	5/2011	Jiang et al.	8,417,491 B2	4/2013	Trovato et al.
7,942,852 B2	5/2011	Mas et al.	8,449,465 B2	5/2013	Nair et al.
7,947,012 B2	5/2011	Spurchise et al.	8,454,685 B2	6/2013	Hariton et al.
7,951,186 B2	5/2011	Eidenschink et al.	8,454,686 B2	6/2013	Alkhatib
7,952,719 B2	5/2011	Brennan, III	8,475,522 B2	7/2013	Jimenez et al.
7,972,353 B2	7/2011	Hendriksen et al.	8,478,384 B2	7/2013	Schmitt et al.
7,976,492 B2	7/2011	Brauker et al.	8,486,062 B2	7/2013	Belhe et al.
7,977,950 B2	7/2011	Maslen	8,486,063 B2	7/2013	Werneth et al.
7,978,916 B2	7/2011	Klingensmith et al.	8,491,567 B2	7/2013	Magnin et al.
7,981,041 B2	7/2011	McGahan	8,500,798 B2	8/2013	Rowe et al.
7,981,151 B2	7/2011	Rowe	8,500,798 B2	8/2013	Rowe et al.
7,983,737 B2	7/2011	Feldman et al.	8,550,911 B2	10/2013	Sylla
7,993,333 B2	8/2011	Oral et al.	8,594,757 B2	11/2013	Boppart et al.
7,995,210 B2	8/2011	Tearney et al.	8,597,349 B2	12/2013	Alkhatib
7,996,060 B2	8/2011	Trofimov et al.	8,600,477 B2	12/2013	Beyar et al.
7,999,938 B2	8/2011	Wang	8,600,917 B1	12/2013	Schimert et al.
8,021,377 B2	9/2011	Eskuri	8,601,056 B2	12/2013	Lauwers et al.
8,021,420 B2	9/2011	Dolan	8,620,055 B2	12/2013	Barratt et al.
8,036,732 B2	10/2011	Milner	8,644,910 B2	2/2014	Rouso et al.
8,040,586 B2	10/2011	Smith et al.	2001/0007940 A1	7/2001	Tu et al.
8,047,996 B2	11/2011	Goodnow et al.	2001/0029337 A1	10/2001	Pantages et al.
8,049,900 B2	11/2011	Kemp et al.	2001/0037073 A1	11/2001	White et al.
8,050,478 B2	11/2011	Li et al.	2001/0046345 A1	11/2001	Snyder et al.
8,050,523 B2	11/2011	Younge et al.	2001/0049548 A1	12/2001	Vardi et al.
8,052,605 B2	11/2011	Muller et al.	2002/0034276 A1	3/2002	Hu et al.
8,057,394 B2	11/2011	Dala-Krishna	2002/0041723 A1	4/2002	Ronnekleiv et al.
8,059,923 B2	11/2011	Bates et al.	2002/0069676 A1	6/2002	Kopp et al.
			2002/0089335 A1	7/2002	Williams
			2002/0099289 A1	7/2002	Crowley
			2002/0163646 A1	11/2002	Anderson
			2002/0186818 A1	12/2002	Arnaud et al.
			2002/0196446 A1	12/2002	Roth et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2002/0197456	A1	12/2002	Pope	2006/0015126	A1	1/2006	Sher
2003/0004412	A1	1/2003	Izatt et al.	2006/0029634	A1	2/2006	Berg et al.
2003/0016604	A1	1/2003	Hanes	2006/0036167	A1	2/2006	Shina
2003/0018273	A1	1/2003	Cori et al.	2006/0038115	A1	2/2006	Maas
2003/0023153	A1	1/2003	Izatt et al.	2006/0039004	A1	2/2006	de Boer et al.
2003/0032886	A1	2/2003	Dgany et al.	2006/0041180	A1	2/2006	Viswanathan et al.
2003/0050871	A1	3/2003	Broughton	2006/0045536	A1	3/2006	Arahira
2003/0065371	A1	4/2003	Satake	2006/0055936	A1	3/2006	Yun et al.
2003/0069723	A1	4/2003	Hegde	2006/0058622	A1	3/2006	Tearney et al.
2003/0077043	A1	4/2003	Hamm et al.	2006/0064009	A1	3/2006	Webler et al.
2003/0085635	A1	5/2003	Davidson	2006/0067620	A1	3/2006	Shishkov et al.
2003/0090753	A1	5/2003	Takeyama et al.	2006/0072808	A1	4/2006	Grimm et al.
2003/0092995	A1	5/2003	Thompson	2006/0074442	A1	4/2006	Noriega et al.
2003/0093059	A1	5/2003	Griffin et al.	2006/0098927	A1	5/2006	Schmidt et al.
2003/0103212	A1	6/2003	Westphal et al.	2006/0100694	A1	5/2006	Globerman
2003/0152259	A1	8/2003	Belykh et al.	2006/0106375	A1	5/2006	Werneth et al.
2003/0181802	A1	9/2003	Ogawa	2006/0132790	A1	6/2006	Gutin
2003/0187369	A1	10/2003	Lewis et al.	2006/0135870	A1	6/2006	Webler
2003/0194165	A1	10/2003	Silberberg et al.	2006/0142703	A1	6/2006	Carter et al.
2003/0195419	A1	10/2003	Harada	2006/0142733	A1	6/2006	Forsberg
2003/0208116	A1	11/2003	Liang et al.	2006/0173299	A1	8/2006	Romley et al.
2003/0212491	A1	11/2003	Mitchell et al.	2006/0179255	A1	8/2006	Yamazaki
2003/0219202	A1	11/2003	Loeb et al.	2006/0184048	A1	8/2006	Saadat
2003/0220749	A1	11/2003	Chen et al.	2006/0187537	A1	8/2006	Huber et al.
2003/0228039	A1	12/2003	Green	2006/0195269	A1	8/2006	Yeatman et al.
2004/0015065	A1	1/2004	Panescu et al.	2006/0204119	A1	9/2006	Feng et al.
2004/0023317	A1	2/2004	Motamedi et al.	2006/0229591	A1	10/2006	Lee
2004/0028333	A1	2/2004	Lomas	2006/0239312	A1	10/2006	Kewitsch et al.
2004/0037742	A1	2/2004	Jen et al.	2006/0241342	A1	10/2006	Macaulay et al.
2004/0042066	A1	3/2004	Kinoshita et al.	2006/0241465	A1	10/2006	Huennekens et al.
2004/0054287	A1	3/2004	Stephens	2006/0241503	A1	10/2006	Schmitt et al.
2004/0067000	A1	4/2004	Bates et al.	2006/0244973	A1	11/2006	Yun et al.
2004/0068161	A1	4/2004	Couvillon	2006/0258895	A1	11/2006	Maschke
2004/0082844	A1	4/2004	Vardi et al.	2006/0264743	A1	11/2006	Kleen
2004/0092830	A1	5/2004	Scott et al.	2006/0267756	A1	11/2006	Kates
2004/0106853	A1	6/2004	Moriyama	2006/0270976	A1	11/2006	Savage et al.
2004/0111552	A1	6/2004	Arimilli et al.	2006/0276709	A1	12/2006	Khamene et al.
2004/0126048	A1	7/2004	Dave et al.	2006/0279742	A1	12/2006	Tearney et al.
2004/0143160	A1	7/2004	Couvillon	2006/0279743	A1	12/2006	Boesser et al.
2004/0146546	A1	7/2004	Gravett et al.	2006/0285638	A1	12/2006	Boese et al.
2004/0186369	A1	9/2004	Lam	2006/0287595	A1	12/2006	Maschke
2004/0186558	A1	9/2004	Pavcnik et al.	2006/0293597	A1	12/2006	Johnson et al.
2004/0195512	A1	10/2004	Crosetto	2007/0015969	A1	1/2007	Feldman et al.
2004/0220606	A1	11/2004	Goshgarian	2007/0016029	A1	1/2007	Donaldson et al.
2004/0225220	A1	11/2004	Rich	2007/0016034	A1	1/2007	Donaldson
2004/0239938	A1	12/2004	Izatt	2007/0016062	A1	1/2007	Park et al.
2004/0242990	A1	12/2004	Brister et al.	2007/0027390	A1	2/2007	Maschke et al.
2004/0248439	A1	12/2004	Gernhardt et al.	2007/0036417	A1	2/2007	Argiro et al.
2004/0260236	A1	12/2004	Manning et al.	2007/0038061	A1	2/2007	Huennekens et al.
2005/0013778	A1	1/2005	Green et al.	2007/0038121	A1	2/2007	Feldman et al.
2005/0031176	A1	2/2005	Hertel et al.	2007/0038125	A1	2/2007	Kleen et al.
2005/0036150	A1	2/2005	Izatt et al.	2007/0043292	A1	2/2007	Camus et al.
2005/0078317	A1	4/2005	Law et al.	2007/0043597	A1	2/2007	Donaldson
2005/0101859	A1	5/2005	Maschke	2007/0049847	A1	3/2007	Osborne
2005/0123180	A1	6/2005	Luo	2007/0060973	A1	3/2007	Ludvig et al.
2005/0140582	A1	6/2005	Lee et al.	2007/0065077	A1	3/2007	Childers et al.
2005/0140682	A1	6/2005	Sumanaweera et al.	2007/0066888	A1	3/2007	Maschke
2005/0140981	A1	6/2005	Waelti	2007/0066890	A1	3/2007	Maschke
2005/0140984	A1	6/2005	Hitzenberger	2007/0066983	A1	3/2007	Maschke
2005/0147303	A1	7/2005	Zhou et al.	2007/0084995	A1	4/2007	Newton et al.
2005/0165439	A1	7/2005	Weber et al.	2007/0100226	A1	5/2007	Yankelevitz et al.
2005/0171433	A1	8/2005	Boppart et al.	2007/0135887	A1	6/2007	Maschke
2005/0171438	A1	8/2005	Chen et al.	2007/0142707	A1	6/2007	Wiklof et al.
2005/0182297	A1	8/2005	Gravenstein et al.	2007/0156019	A1	7/2007	Larkin et al.
2005/0196028	A1	9/2005	Kleen et al.	2007/0161893	A1	7/2007	Milner et al.
2005/0197585	A1	9/2005	Brockway et al.	2007/0161896	A1	7/2007	Adachi et al.
2005/0213103	A1	9/2005	Everett et al.	2007/0161963	A1	7/2007	Smalling
2005/0215942	A1	9/2005	Abrahamson et al.	2007/0162860	A1	7/2007	Muralidharan et al.
2005/0234445	A1	10/2005	Conquergood et al.	2007/0165141	A1	7/2007	Srinivas et al.
2005/0243322	A1	11/2005	Lasker et al.	2007/0167710	A1	7/2007	Unal et al.
2005/0249391	A1	11/2005	Kimmel et al.	2007/0167804	A1	7/2007	Park et al.
2005/0251567	A1	11/2005	Ballew et al.	2007/0191682	A1	8/2007	Rolland et al.
2005/0254059	A1	11/2005	Alphonse	2007/0201736	A1	8/2007	Klingensmith et al.
2005/0264823	A1	12/2005	Zhu et al.	2007/0206193	A1	9/2007	Pesach
2006/0013523	A1	1/2006	Childers et al.	2007/0208276	A1	9/2007	Komkven Volk et al.
				2007/0225220	A1	9/2007	Ming et al.
				2007/0225590	A1	9/2007	Ramos
				2007/0229801	A1	10/2007	Tearney et al.
				2007/0232872	A1	10/2007	Prough et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0232874	A1	10/2007	Ince	2009/0138544	A1	5/2009	Wegenkittl et al.
2007/0232890	A1	10/2007	Hirota	2009/0149739	A9	6/2009	Maschke
2007/0232891	A1	10/2007	Hirota	2009/0156941	A1	6/2009	Moore
2007/0232892	A1	10/2007	Hirota	2009/0174886	A1	7/2009	Inoue
2007/0232893	A1	10/2007	Tanioka	2009/0174931	A1	7/2009	Huber et al.
2007/0232933	A1	10/2007	Gille et al.	2009/0177090	A1	7/2009	Grunwald et al.
2007/0238957	A1	10/2007	Yared	2009/0177183	A1	7/2009	Pinkernell et al.
2007/0239395	A1	10/2007	Jenkins	2009/0195514	A1	8/2009	Glynn et al.
2007/0247033	A1	10/2007	Eidenschink et al.	2009/0196470	A1	8/2009	Carl et al.
2007/0249967	A1*	10/2007	Buly A61B 5/1121 600/595	2009/0198125	A1	8/2009	Nakabayashi et al.
2007/0250000	A1	10/2007	Magnin et al.	2009/0203991	A1	8/2009	Papaioannou et al.
2007/0250036	A1	10/2007	Volk et al.	2009/0264768	A1	10/2009	Courtney et al.
2007/0258094	A1	11/2007	Izatt et al.	2009/0269014	A1	10/2009	Winberg et al.
2007/0260138	A1	11/2007	Feldman et al.	2009/0270695	A1	10/2009	McEowen
2007/0278389	A1	12/2007	Ajgaonkar et al.	2009/0284322	A1	11/2009	Harrison et al.
2007/0287914	A1	12/2007	Cohen	2009/0284332	A1	11/2009	Moore et al.
2008/0002183	A1	1/2008	Yatagai et al.	2009/0284749	A1	11/2009	Johnson et al.
2008/0013093	A1	1/2008	Izatt et al.	2009/0290167	A1	11/2009	Flanders et al.
2008/0021275	A1	1/2008	Tearney et al.	2009/0292048	A1	11/2009	Li et al.
2008/0027481	A1	1/2008	Gilson et al.	2009/0299195	A1	12/2009	Muller et al.
2008/0043024	A1	2/2008	Schiwietz et al.	2009/0299284	A1	12/2009	Holman et al.
2008/0045842	A1	2/2008	Furnish	2009/0318951	A1	12/2009	Kashkarov et al.
2008/0051660	A1	2/2008	Kakadaris et al.	2009/0326634	A1	12/2009	Vardi
2008/0063304	A1	3/2008	Russak	2010/0007669	A1	1/2010	Bethune et al.
2008/0085041	A1	4/2008	Breeuwer	2010/0030042	A1	2/2010	Denninghoff et al.
2008/0095465	A1	4/2008	Mullick et al.	2010/0061611	A1	3/2010	Xu et al.
2008/0095714	A1	4/2008	Castella et al.	2010/0063400	A1	3/2010	Hall et al.
2008/0097194	A1	4/2008	Milner	2010/0087732	A1	4/2010	Eberle et al.
2008/0101667	A1	5/2008	Begelman et al.	2010/0094125	A1	4/2010	Younge et al.
2008/0108867	A1	5/2008	Zhou	2010/0094127	A1	4/2010	Xu
2008/0114254	A1	5/2008	Matcovitch et al.	2010/0094135	A1	4/2010	Fang-Yen et al.
2008/0119739	A1	5/2008	Vardi et al.	2010/0094143	A1	4/2010	Mahapatra et al.
2008/0124495	A1	5/2008	Horn et al.	2010/0113919	A1	5/2010	Maschke
2008/0125772	A1	5/2008	Stone et al.	2010/0125238	A1	5/2010	Lye et al.
2008/0139897	A1	6/2008	Ainsworth et al.	2010/0125268	A1	5/2010	Gustus et al.
2008/0143707	A1	6/2008	Mitchell	2010/0125648	A1	5/2010	Zaharia et al.
2008/0146941	A1	6/2008	Dala-Krishna	2010/0128348	A1	5/2010	Taverner
2008/0147111	A1	6/2008	Johnson et al.	2010/0152717	A1	6/2010	Keeler
2008/0154128	A1	6/2008	Milner	2010/0160788	A1	6/2010	Davies et al.
2008/0161696	A1	7/2008	Schmitt et al.	2010/0161023	A1	6/2010	Cohen et al.
2008/0171944	A1	7/2008	Brenneman et al.	2010/0168714	A1	7/2010	Burke et al.
2008/0175465	A1	7/2008	Jiang et al.	2010/0179421	A1	7/2010	Tupin
2008/0177183	A1	7/2008	Courtney	2010/0179426	A1	7/2010	Davies et al.
2008/0180683	A1	7/2008	Kemp	2010/0220334	A1	9/2010	Condit et al.
2008/0181477	A1	7/2008	Izatt et al.	2010/0226607	A1	9/2010	Zhang et al.
2008/0183075	A1	7/2008	Govari	2010/0234736	A1	9/2010	Corl
2008/0187201	A1	8/2008	Liang et al.	2010/0249601	A1	9/2010	Courtney
2008/0228086	A1	9/2008	Ilegbusi et al.	2010/0253949	A1	10/2010	Adler
2008/0247622	A1	10/2008	Aylward et al.	2010/0256616	A1	10/2010	Katoh et al.
2008/0247716	A1	10/2008	Thomas et al.	2010/0272432	A1	10/2010	Johnson
2008/0262470	A1	10/2008	Lee et al.	2010/0284590	A1	11/2010	Peng et al.
2008/0262489	A1	10/2008	Steinke	2010/0290693	A1	11/2010	Cohen et al.
2008/0269599	A1	10/2008	Csavoy et al.	2010/0331950	A1	12/2010	Strommer
2008/0281205	A1	11/2008	Naghavi et al.	2011/0010925	A1	1/2011	Nix et al.
2008/0281248	A1	11/2008	Angheloiu et al.	2011/0021926	A1	1/2011	Spencer et al.
2008/0285043	A1	11/2008	Fercher et al.	2011/0025853	A1	2/2011	Richardson
2008/0287795	A1	11/2008	Klingensmith et al.	2011/0026797	A1	2/2011	Declerck et al.
2008/0291463	A1	11/2008	Milner et al.	2011/0032533	A1	2/2011	Izatt et al.
2008/0292173	A1	11/2008	Hsieh et al.	2011/0034801	A1	2/2011	Baumgart
2008/0294034	A1	11/2008	Krueger et al.	2011/0044546	A1	2/2011	Pan et al.
2008/0298655	A1	12/2008	Edwards	2011/0066073	A1	3/2011	Kuiper et al.
2008/0306766	A1	12/2008	Ozeki et al.	2011/0071401	A1	3/2011	Hastings et al.
2009/0009801	A1	1/2009	Tabuki	2011/0072405	A1	3/2011	Chen et al.
2009/0018393	A1	1/2009	Dick et al.	2011/0077528	A1	3/2011	Kemp et al.
2009/0034813	A1	2/2009	Dikmen et al.	2011/0080591	A1	4/2011	Johnson et al.
2009/0043191	A1	2/2009	Castella et al.	2011/0087104	A1	4/2011	Moore et al.
2009/0046295	A1	2/2009	Kemp et al.	2011/0137140	A1	6/2011	Tearney et al.
2009/0052614	A1	2/2009	Hempel et al.	2011/0144502	A1	6/2011	Zhou et al.
2009/0069843	A1	3/2009	Agnew	2011/0152771	A1	6/2011	Milner et al.
2009/0079993	A1	3/2009	Yatagai et al.	2011/0157597	A1	6/2011	Lu et al.
2009/0088650	A1	4/2009	Cori	2011/0160586	A1	6/2011	Li et al.
2009/0093980	A1	4/2009	Kemp et al.	2011/0178413	A1	7/2011	Schmitt et al.
2009/0122320	A1*	5/2009	Petersen A61B 5/6852 359/896	2011/0190586	A1	8/2011	Kemp
				2011/0191084	A1	8/2011	Cooke
				2011/0216378	A1	9/2011	Poon et al.
				2011/0220985	A1	9/2011	Son et al.
				2011/0238061	A1	9/2011	van der Weide et al.
				2011/0238083	A1	9/2011	Moll et al.
				2011/0245669	A1	10/2011	Zhang

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0249094 A1 10/2011 Wang et al.
 2011/0257545 A1 10/2011 Suri
 2011/0264125 A1 10/2011 Wilson et al.
 2011/0274329 A1 11/2011 Mathew et al.
 2011/0282334 A1 11/2011 Groenhoff
 2011/0301684 A1 12/2011 Fischell et al.
 2011/0306995 A1 12/2011 Moberg
 2011/0319752 A1 12/2011 Steinberg et al.
 2012/0004529 A1 1/2012 Tolkowsky et al.
 2012/0004668 A1 1/2012 Wallace et al.
 2012/0013914 A1 1/2012 Kemp et al.
 2012/0016344 A1 1/2012 Kusakabe
 2012/0016395 A1 1/2012 Olson
 2012/0022360 A1 1/2012 Kemp
 2012/0026503 A1 2/2012 Lewandowski et al.
 2012/0029007 A1 2/2012 Graham et al.
 2012/0059253 A1 3/2012 Wang et al.
 2012/0059368 A1 3/2012 Takaoka et al.
 2012/0062843 A1 3/2012 Ferguson et al.
 2012/0065481 A1 3/2012 Hunter et al.
 2012/0071823 A1 3/2012 Chen
 2012/0071838 A1 3/2012 Fojtik
 2012/0075638 A1 3/2012 Rollins
 2012/0083696 A1 4/2012 Kitamura
 2012/0095340 A1 4/2012 Smith
 2012/0095372 A1 4/2012 Sverdlik et al.
 2012/0108943 A1 5/2012 Bates et al.
 2012/0113108 A1 5/2012 Dala-Krishna
 2012/0116353 A1 5/2012 Arnold et al.
 2012/0130243 A1 5/2012 Balocco et al.
 2012/0130247 A1 5/2012 Waters et al.
 2012/0136259 A1 5/2012 Milner et al.
 2012/0136427 A1 5/2012 Palmaz et al.
 2012/0137075 A1 5/2012 Vorbach
 2012/0155734 A1 6/2012 Barratt et al.
 2012/0158101 A1 6/2012 Stone et al.
 2012/0162660 A1 6/2012 Kemp
 2012/0165661 A1 6/2012 Kemp et al.
 2012/0170848 A1 7/2012 Kemp et al.
 2012/0172698 A1 7/2012 Teo et al.
 2012/0176607 A1 7/2012 Ott
 2012/0184853 A1 7/2012 Waters
 2012/0184859 A1 7/2012 Shah et al.
 2012/0184977 A1 7/2012 Wolf
 2012/0215094 A1 8/2012 Rahimian et al.
 2012/0220836 A1 8/2012 Alpert et al.
 2012/0220851 A1 8/2012 Razansky et al.
 2012/0220865 A1 8/2012 Brown et al.
 2012/0220874 A1 8/2012 Hancock et al.
 2012/0220883 A1 8/2012 Manstrom et al.
 2012/0224751 A1 9/2012 Kemp et al.
 2012/0226153 A1 9/2012 Brown et al.
 2012/0230565 A1 9/2012 Steinberg et al.
 2012/0232400 A1 9/2012 Dickinson et al.
 2012/0238869 A1 9/2012 Schmitt et al.
 2012/0238956 A1 9/2012 Yamada et al.
 2012/0244043 A1 9/2012 Leblanc et al.
 2012/0250028 A1 10/2012 Schmitt et al.
 2012/0253186 A1 10/2012 Simpson et al.
 2012/0253192 A1 10/2012 Cressman
 2012/0253276 A1 10/2012 Govari et al.
 2012/0257210 A1 10/2012 Whitney et al.
 2012/0262720 A1 10/2012 Brown et al.
 2012/0265077 A1 10/2012 Gille et al.
 2012/0265268 A1 10/2012 Blum et al.
 2012/0265296 A1 10/2012 McNamara et al.
 2012/0271170 A1 10/2012 Emelianov et al.
 2012/0271175 A1 10/2012 Moore et al.
 2012/0271339 A1 10/2012 O'Beirne et al.
 2012/0274338 A1 11/2012 Baks et al.
 2012/0276390 A1 11/2012 Ji et al.
 2012/0277722 A1 11/2012 Gerber et al.
 2012/0279764 A1 11/2012 Jiang et al.
 2012/0283758 A1 11/2012 Miller et al.
 2012/0289987 A1 11/2012 Wilson et al.

2012/0299439 A1 11/2012 Huang
 2012/0310081 A1 12/2012 Adler et al.
 2012/0310332 A1 12/2012 Murray et al.
 2012/0319535 A1 12/2012 Dausch
 2012/0323075 A1 12/2012 Younge et al.
 2012/0323127 A1 12/2012 Boyden et al.
 2012/0330141 A1 12/2012 Brown et al.
 2013/0006105 A1* 1/2013 Furuichi A61B 5/0084
 600/427
 2013/0015975 A1 1/2013 Huennekens et al.
 2013/0023762 A1 1/2013 Huennekens et al.
 2013/0023763 A1 1/2013 Huennekens et al.
 2013/0026655 A1 1/2013 Lee et al.
 2013/0030295 A1 1/2013 Huennekens et al.
 2013/0030303 A1 1/2013 Ahmed et al.
 2013/0030410 A1 1/2013 Drasler et al.
 2013/0053949 A1 2/2013 Pintor et al.
 2013/0109958 A1 5/2013 Baumgart et al.
 2013/0109959 A1 5/2013 Baumgart et al.
 2013/0137980 A1 5/2013 Waters et al.
 2013/0150716 A1 6/2013 Stigall et al.
 2013/0158594 A1 6/2013 Carrison et al.
 2013/0218201 A1 8/2013 Obermiller et al.
 2013/0218267 A1 8/2013 Braido et al.
 2013/0223789 A1 8/2013 Lee et al.
 2013/0223798 A1 8/2013 Jenner et al.
 2013/0296704 A1 11/2013 Magnin et al.
 2013/0303907 A1 11/2013 Corl
 2013/0303920 A1 11/2013 Corl
 2013/0310698 A1 11/2013 Judell et al.
 2013/0331820 A1 12/2013 Itou et al.
 2013/0338766 A1 12/2013 Hastings et al.
 2013/0339958 A1 12/2013 Droste et al.
 2014/0039294 A1 2/2014 Jiang
 2014/0180067 A1 6/2014 Stigall et al.
 2014/0180128 A1 6/2014 Corl
 2014/0200438 A1 7/2014 Millett et al.
 2014/0268167 A1* 9/2014 Friedman G01J 9/02
 356/479

FOREIGN PATENT DOCUMENTS

EP 2438877 A2 4/2012
 GB 2280261 A 1/1995
 JP 2000-262461 A 9/2000
 JP 2000-292260 A 10/2000
 JP 2001-125009 A 5/2001
 JP 2001-272331 A 10/2001
 JP 2002-374034 A 12/2002
 JP 2003-143783 A 5/2003
 JP 2003-172690 A 6/2003
 JP 2003-256876 A 9/2003
 JP 2003-287534 A 10/2003
 JP 2005-274380 A 10/2005
 JP 2006-184284 A 7/2006
 JP 2006-266797 A 10/2006
 JP 2006-313158 A 11/2006
 JP 2007-024677 A 2/2007
 JP 2009-233001 A 10/2009
 JP 2011-56786 A 3/2011
 WO 91/01156 A1 2/1991
 WO 92/16865 A1 10/1992
 WO 93/06213 A1 4/1993
 WO 93/08829 A1 5/1993
 WO 98/38907 A1 9/1998
 WO 98/57583 A1 12/1998
 WO 00/11511 A1 3/2000
 WO 00/044296 A1 8/2000
 WO 01/11409 A2 2/2001
 WO 03/062802 A2 7/2003
 WO 03/073950 A1 9/2003
 WO 2004/010856 A1 2/2004
 WO 2004/023992 A1 3/2004
 WO 2004/096049 A2 11/2004
 WO 2005/047813 A1 5/2005
 WO 2005/106695 A2 11/2005
 WO 2006/029634 A2 3/2006
 WO 2006/037132 A1 4/2006
 WO 2006/039091 A2 4/2006

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	2006/061829	A1	6/2006
WO	2006/068875	A2	6/2006
WO	2006/111704	A1	10/2006
WO	2006/119416	A2	11/2006
WO	2006/121851	A1	11/2006
WO	2006/130802	A2	12/2006
WO	2007/002685	A2	1/2007
WO	2007/025230	A2	3/2007
WO	2007/045690	A1	4/2007
WO	2007/058895	A2	5/2007
WO	2007/067323	A2	6/2007
WO	2007/084995	A2	7/2007
WO	2008/058084	A2	5/2008
WO	2008/069991	A1	6/2008
WO	2008/107905	A2	9/2008
WO	2009/009799	A1	1/2009
WO	2009/009801	A1	1/2009
WO	2009/046431	A1	4/2009
WO	2009/121067	A1	10/2009
WO	2009/137704	A1	11/2009
WO	2011/06886	A2	1/2011
WO	2011/038048	A1	3/2011
WO	2011/081688	A1	7/2011
WO	2012/003369	A2	1/2012
WO	2012/061935	A1	5/2012
WO	2012/071388	A2	5/2012
WO	2012/087818	A1	6/2012
WO	2012/098194	A1	7/2012
WO	2012/109676	A1	8/2012
WO	2012/130289	A1	10/2012
WO	2012/154767	A2	11/2012
WO	2012/155040	A1	11/2012
WO	2013/033414	A1	3/2013
WO	2013/033415	A2	3/2013
WO	2013/033418	A1	3/2013
WO	2013/033489	A1	3/2013
WO	2013/033490	A1	3/2013
WO	2013/033592	A1	3/2013
WO	2013/126390	A1	8/2013
WO	2014/109879	A1	7/2014

OTHER PUBLICATIONS

Liew, Yih Miin, et al. "Reduction of image artifacts in three-dimensional optical coherence tomography of skin in vivo." *Journal of biomedical optics* 16.11 (2011): 116018-116018. (Year: 2011).*

Westphal, Volker, et al. "Correction of geometric and refractive image distortions in optical coherence tomography applying Fermat's principle." *Optics express* 10.9 (2002): 397-404. (Year: 2002).*

Bell, Malcolm R. et al "Validation of a new UNIX based Quantitative Coronary Angiographic System for the Measurement of Coronary Artery Lesions" *Catheterization and Cardiovascular Diagnosis*, vol. 40.1, 1997, pp. 66-74.

Tommasini, Giorgio et al "A Deterministic Approach to Automated Stenosis Quantification", *Catheterization and Cardiovascular Interventions*, vol. 48.4, 1999, pp. 435-445.

Sihan et al., 2008, A novel approach to quantitative analysis of intraluminal optical coherence tomography imaging, *Comput. Cardiol*:1089-1092.

Siwy et al., 2003, Electro-responsive asymmetric nanopores in polyimide with stable ion-current signal, *Applied Physics A: Materials Science & Processing* 76:781-785.

Smith et al., 1989, Absolute displacement measurements using modulation of the spectrum of white light in a Michelson interferometer, *Applied Optics*, 28(16):3339-3342.

Smith, 1997, *The Scientist and Engineer's Guide to Digital Signal Processing*, California Technical Publishing, San Diego, CA:432-436.

Soller, 2003, Polarization diverse optical frequency domain interferometry: All coupler implementation, Bragg Grating, Photosensitivity, and Poling in Glass Waveguides Conference MB4:30-32.

Song et al., 2012, Active tremor cancellation by a "Smart" handheld vitreoretinal microsurgical tool using swept source optical coherence tomography, *Optics Express*, 20(21):23414-23421.

Stenqvist et al., 1983, Stiffness of central venous catheters, *Acta Anaesthesiol Scand.*, 2:153-157.

Strickland, 1970, *Time-Domain Reflectometer Measurements*, Tektronix, Beaverton, OR, (107 pages).

Strobl et al., 2009, An Introduction to Recursive Partitioning: Rationale, Application and Characteristics of Classification and Regression Trees, *Bagging and Random Forests, Psychol Methods.*, 14(4):323-348.

Sutcliffe et al., 1986, Dynamics of UV laser ablation of organic polymer surfaces, *Journal of Applied Physics*, 60(9):3315-3322.

Suzuki, 2013, A novel guidewire approach for handling acute-angle bifurcations, *J Inv Cardiol* 25(1):48-54.

Tanimoto et al., 2008, A novel approach for quantitative analysis of intracoronary optical coherence tomography: high inter-observer agreement with computer-assisted contour detection, *Cathet Cardiovascular Intervent.*, 72(2):228-235.

Tearney et al., 1997, In vivo Endoscopic Optical Biopsy with Optical Coherence Tomography, *Science*, 276:2037-2039.

Tonino et al., 2009, Fractional flow reserve versus angiography for guiding percutaneous coronary intervention, *The New England Journal of Medicine*, 360:213-224.

Toregeani et al., 2008, Evaluation of hemodialysis arteriovenous fistula maturation by color-flow Doppler ultrasound, *J Vasc. Bras.* 7(3):203-213.

Translation of Notice of Reason(s) for Refusal dated Apr. 30, 2014, for Japanese Patent Application No. 2011-508677, (5 pages).

Translation of Notice of Reason(s) for Refusal dated May 25, 2012, for Japanese Patent Application No. 2009-536425, (3 pages).

Translation of Notice of Reason(s) for Refusal dated Nov. 22, 2012, for Japanese Patent Application No. 2010-516304, (6 pages).

Trauneker et al., 1991, Bispecific single chain molecules (Janusins) target cytotoxic lymphocytes on HIV infected cells *EMBO J.*, 10:3655-3659.

Trolier-McKinstry et al., 2004, Thin Film Piezoelectric for MEMS, *Journal of Electroceramics* 12:7-17.

Tuniz et al., 2010, Weaving the invisible thread: design of an optically invisible metamaterial fibre, *Optics Express* 18(17):18095-18105.

Turk et al., 1991, Eigenfaces for Recognition, *Journal of Cognitive Neuroscience* 3(1):71-86.

Tuzel et al., 2006, Region Covariance: A Fast Descriptor for Detection and Classification, *European Conference on Computer Vision (ECCV)*.

Urban et al., 2010, Design of a Pressure Sensor Based on Optical Bragg Grating Lateral Deformation, *Sensors (Basel)*, 10(12):11212-11225.

Vakhtin et al., 2003, Common-path interferometer for frequency-domain optical coherence tomography, *Applied Optics*, 42(34):6953-6958.

Vakoc et al., 2005, Phase-Resolved Optical Frequency Domain Imaging, *Optics Express* 13(14):5483-5493.

Verhoeyen et al., 1988, Reshaping human antibodies: grafting an antilysozyme activity, *Science*, 239:1534-1536.

Villard et al., 2002, Use of a blood substitute to determine instantaneous murine right ventricular thickening with optical coherence tomography, *Circulation*, 105:1843-1849.

Wang et al., 2002, Optimizing the Beam Pattern of a Forward-Viewing Ring-Annular Ultrasound Array for Intravascular Imaging, *Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, 49(12).

Wang et al., 2006, Multiple biomarkers for the prediction of first major cardiovascular events and death, *The New England Journal of Medicine*, 355(25):2631-2639.

Wang et al., 2009, Robust Guidewire Tracking in Fluoroscopy, *IEEE Conference on Computer Vision and Pattern Recognition—CVPR 2009*:691-698.

Wang et al., 2011, In vivo intracardiac optical coherence tomography imaging through percutaneous access: toward image-guided radio-frequency ablation, *J. Biomed. Opt.* 0001 16(11):110505-1 (3 pages).

(56)

References Cited

OTHER PUBLICATIONS

- Waterhouse et al., 1993, Combinatorial infection and in vivo recombination: a strategy for making large phage antibody repertoires, *Nucleic Acids Res.*, 21:2265-2266.
- Wegener, 2011, 3D Photonic Metamaterials and Invisibility Cloaks: The Method of Making, MEMS 2011, Cancun, Mexico, Jan. 23-27, 2011.
- West et al., 1991, Arterial insufficiency in hemodialysis access procedures: correction by banding technique, *Transpl Proc* 23(2):1838-40.
- Wyawahare et al., 2009, Image registration techniques: an overview, *International Journal of Signal Processing, Image Processing and Pattern Recognition*, 2(3):11-28.
- Yaqoob et al., 2006, Methods and application areas of endoscopic optical coherence tomography, *J. Biomed. Opt.*, 11, 063001-1-063001-19.
- Yasuno et al., 2004, Polarization-sensitive complex Fourier domain optical coherence tomography for Jones matrix imaging of biological samples, *Applied Physics Letters* 85(15):3023-3025.
- Zhang et al., 2004, Full range polarization-sensitive Fourier domain optical coherence tomography, *Optics Express*, 12(24):6033-6039.
- Zitova et al., 2003, Image registration methods: A survey. *Image and Vision Computing*, 21(11):977-1000.
- Little et al., 1991, The underlying coronary lesion in myocardial infarction: implications for coronary angiography, *Clinica Cardiologia*, 14(11):868-874.
- Loo, 2004, Nanoshell Enabled Photonics-Based Imaging and Therapy of Cancer, *Technology in Cancer Research & Treatment* 3(1):33-40. Machine translation of JP 2000-097846.
- Machine translation of JP 2000-321034.
- Machine translation of JP 2000-329534.
- Machine translation of JP 2004-004080.
- Maintz et al., 1998, An Overview of Medical Image Registration Methods, Technical Report UU-CS, (22 pages).
- Mamas et al., 2010, Resting Pd/Pa measured with intracoronary pressure wire strongly predicts fractional flow reserve, *Journal of Invasive Cardiology* 22(6):260-265.
- Marks et al., 1991, By-passing Immunization Human Antibodies from V-gene Libraries Displayed on Phage, *J. Mol. Biol.* 222:581-597.
- Marks et al., 1992, By-Passing Immunization: Building High Affinity Human Antibodies by Chain Shuffling, *BioTechnol.*, 10:779-783.
- Maruno et al., 1991, Fluorine containing optical adhesives for optical communications systems, *J. Appl. Polymer. Sci.* 42:2141-2148.
- McCafferty et al., 1990, Phage antibodies: filamentous phage displaying antibody variable domains, *Nature* 348:552-554.
- Mendieta et al., 1996, Complementary sequence correlations with applications to reflectometry studies, *Instrumentation and Development* 3(6):37-46.
- Mickley, 2008, Steal Syndrome-strategies to preserve vascular access and extremity, *Nephrol Dial Transplant* 23:19-24.
- Miller et al., 2010, The Miller banding procedure is an effective method for treating dialysis-associated steal syndrome, *Kidney International* 77:359-366.
- Milstein et al., 1983, Hybrid hybridomas and their use in immunohistochemistry, *Nature* 305:537-540.
- Mindlin et al., 1936, A force at a point of a semi-infinite solid, *Physics*, 7:195-202.
- Morrison et al., 1984, Chimeric human antibody molecules: mouse antigen-binding domains with human constant region domains, *PNAS* 81:6851-6855.
- Munson et al., 1980, Ligand: a versatile computerized approach for characterization of ligand-binding systems, *Analytical Biochemistry*, 107:220-239.
- Nezam, 2008, High Speed Polygon-Scanner-Based Wavelength-Swept Laser Source in the Telescope-Less Configurations with Application in Optical Coherence Tomography, *Optics Letters* 33(15):1741-1743.
- Nissen, 2001, Coronary Angiography and Intravascular Ultrasound, *American Journal of Cardiology*, 87(suppl):15A-20A.
- Nitenberg et al., 1995, Coronary vascular reserve in humans: a critical review of methods of evaluation and of interpretation of the results, *Eur Heart J.* 16(Suppl 1):7-21.
- Notice of Reason(s) for Refusal dated Apr. 30, 2013, for Japanese Patent Application No. 2011-508677 for Optical Imaging Catheter for Aberation Balancing to Volcano Corporation, which application is a Japanese national stage entry of PCT/US2009/043181 with international filing date May 7, 2009, of the same title, published on Nov. 12, 2009, as WO 2009/137704, and accompanying English translation of the Notice of Reason(s) for Refusal and machine translations of JP11-56786 and JP2004-290548 (56 pages).
- Nygren, 1982, Conjugation of horseradish peroxidase to Fab fragments with different homobifunctional and heterobifunctional cross-linking reagents. A comparative study, *J. Histochem. and Cytochem.* 30:407-412.
- Oesterle et al., 1986, Angioplasty at coronary bifurcations: single-guide, two-wire technique, *Cathet Cardiovasc Diagn.*, 12:57-63.
- Okuno et al., 2003, Recent Advances in Optical Switches Using Silica-based PLC Technology, *NTT Technical Review* 1(7):20-30.
- Oldenburg et al., 1998, Nanoengineering of Optical Resonances, *Chemical Physics Letters* 288:243-247.
- Oldenburg et al., 2003, Fast-Fourier-Domain Delay Line for In Vivo Optical Coherence Tomography with a Polygonal Scanner, *Applied Optics*, 42(22):4606-4611.
- Othonos, 1997, Fiber Bragg gratings, *Review of Scientific Instruments* 68(12):4309-4341.
- Owens et al., 2007, A Survey of General-Purpose Computation on Graphics Hardware, *Computer Graphics Forum* 26(1):80-113.
- Pain et al., 1981, Preparation of protein A-peroxidase mono conjugate using a heterobifunctional reagent, and its use in enzyme immunoassays, *J Immunol Methods*, 40:219-30.
- Park et al., 2005, Real-time fiber-based multi-functional spectral-domain optical coherence tomography at 1.3 μm ., *Optics Express* 13(11):3931-3944.
- Pasquesi et al., 2006, In vivo detection of exercise induced ultrastructural changes in genetically-altered murine skeletal muscle using polarization-sensitive optical coherence tomography, *Optics Express* 14(4):1547-1556.
- Pepe et al., 2004, Limitations of the odds ratio in gauging the performance of a diagnostic, prognostic, or screening marker, *American Journal of Epidemiology* 159(9):882-890.
- Persson et al., 1985, Acoustic impedance matching of medical ultrasound transducers, *Ultrasonics*, 23(2):83-89.
- Placht et al., 2012, Fast time-of-flight camera based surface registration for radiotherapy patient positioning, *Medical Physics* 39(1):4-17.
- Rabbani et al., 1999, Review: Strategies to achieve coronary arterial plaque stabilization, *Cardiovascular Research* 41:402-417.
- Radvany et al., 2008, Plaque Excision in Management of Lower Extremity Peripheral Arterial Disease with the SilverHawk Atherectomy Catheter, *Seminars in Interventional Radiology*, 25(1):11-19.
- Reddy et al., 1996, An FFT-Based Technique for Translation, Rotation, and Scale-Invariant Image Registration, *IEEE Transaction on Image Processing* 5(8):1266-1271.
- Riechmann et al., 1988, Reshaping human antibodies for therapy, *Nature*, 332:323-327.
- Rivers et al., 1992, Correction of steal syndrome secondary to hemodialysis access fistulas: a simplified quantitative technique, *Surgery*, 112(3):593-7.
- Robbin et al., 2002, Hemodialysis Arteriovenous Fistula Maturity: US Evaluation, *Radiology* 225:59-64.
- Rollins et al., 1998, In vivo video rate optical coherence tomography, *Optics Express* 3:219-229.
- Sarunic et al., 2005, Instantaneous Complex Conjugate Resolved Spectral Domain and Swept-Source OCT Using 3x3 Fiber Couplers, *Optics Express* 13(3):957-967.
- Satiani et al., 2009, Predicted Shortage of Vascular Surgeons in the United States, *J. Vascular Surgery* 50:946-952.
- Schneider et al., 2006, T-banding: A technique for flow reduction of a hyper-functioning arteriovenous fistula, *J Vase Surg.* 43(2):402-405.

(56)

References Cited

OTHER PUBLICATIONS

Sen et al., 2012, Development and validation of a new adenosine-independent index of stenosis severity from coronary wave-intensity analysis, *Journal of the American College of Cardiology* 59(15):1392-1402.

Setta et al., 2005, Soft versus firm embryo transfer catheters for assisted reproduction: a systematic review and meta-analysis, *Human Reproduction*, 20(11):3114-3121.

Seward et al., 1996, Ultrasound Cardioscopy: Embarking on New Journey, *Mayo Clinic Proceedings* 71(7):629-635.

Shen et al., 2006, Eigengene-based linear discriminant model for tumor classification using gene expression microarray data, *Bioinformatics* 22(21):2635-2642.

International Search Report and Written Opinion dated Nov. 2, 2012, for International Patent Application No. PCT/US12/53168, filed Aug. 30, 2013 (8 pages).

International Search Report and Written Opinion dated Apr. 14, 2014, for International Patent Application No. PCT/US2013/076148, filed Dec. 18, 2013 (8 pages).

International Search Report and Written Opinion dated Apr. 21, 2014, for International Patent Application No. PCT/US2013/076015, filed Dec. 18, 2013 (7 pages).

International Search Report and Written Opinion dated Apr. 23, 2014, for International Patent Application No. PCT/US2013/075328, filed Dec. 16, 2013 (8 pages).

International Search Report and Written Opinion dated Apr. 29, 2014, for International Patent Application No. PCT/US13/76093, filed Dec. 18, 2013 (6 pages).

International Search Report and Written Opinion dated Apr. 9, 2014, for International Patent Application No. PCT/US13/75089, filed Dec. 13, 2013 (7 pages).

International Search Report and Written Opinion dated Feb. 21, 2014, for International Patent Application No. PCT/US13/76053, filed Dec. 18, 2013 (9 pages).

International Search Report and Written Opinion dated Feb. 21, 2014, for International Patent Application No. PCT/US2013/076965, filed Dec. 20, 2013 (6 pages).

International Search Report and Written Opinion dated Feb. 27, 2014, for International Patent Application No. PCT/US13/75416, filed Dec. 16, 2013 (7 pages).

International Search Report and Written Opinion dated Feb. 28, 2014, for International Patent Application No. PCT/US13/75653, filed Dec. 17, 2013 (7 pages).

International Search Report and Written Opinion dated Feb. 28, 2014, for International Patent Application No. PCT/US13/75990, filed Dec. 18, 2013 (7 pages).

International Search Report and Written Opinion dated Jan. 16, 2009, for International Patent Application No. PCT/US08/78963 filed on Oct. 6, 2008 (7 Pages).

International Search Report and Written Opinion dated Jul. 30, 2014, for International Patent Application No. PCT/US14/21659, filed Mar. 7, 2014 (15 pages).

International Search Report and Written Opinion dated Mar. 10, 2014, for International Patent Application No. PCT/US2013/076212, filed Dec. 18, 2013 (8 pages).

International Search Report and Written Opinion dated Mar. 11, 2014, for International Patent Application No. PCT/US13/76173, filed Dec. 16, 2013 (9 pages).

International Search Report and Written Opinion dated Mar. 11, 2014, for International Patent Application No. PCT/US13/76449, filed Dec. 19, 2013 (9 pages).

International Search Report and Written Opinion dated Mar. 18, 2014, for International Patent Application No. PCT/US2013/076502, filed Dec. 19, 2013 (7 pages).

International Search Report and Written Opinion dated Mar. 18, 2014, for International Patent Application No. PCT/US2013/076788, filed Dec. 20, 2013 (7 pages).

International Search Report and Written Opinion dated Mar. 19, 2014, for International Patent Application No. PCT/US13/75349, filed Dec. 16, 2013 (10 pages).

International Search Report and Written Opinion dated Mar. 19, 2014, for International Patent Application No. PCT/US2013/076587, filed Dec. 19, 2013 (10 pages).

International Search Report and Written Opinion dated Mar. 19, 2014, for International Patent Application No. PCT/US2013/076909, filed Dec. 20, 2013 (7 pages).

International Search Report and Written Opinion dated Mar. 7, 2014, for International Patent Application No. PCT/US2013/076304, filed Dec. 18, 2013 (9 pages).

International Search Report and Written Opinion dated Mar. 7, 2014, for International Patent Application No. PCT/US2013/076480, filed Dec. 19, 2013 (8 pages).

International Search Report and Written Opinion dated Mar. 7, 2014, for International Patent Application No. PCT/US2013/076512, filed Dec. 19, 2013 (8 pages).

International Search Report and Written Opinion dated Mar. 7, 2014, for International Patent Application No. PCT/US2013/076531, filed Dec. 19, 2013 (10 pages).

Jakobovits et al., 1993, Analysis of homozygous mutant chimeric mice deletion of the immunoglobulin heavy-chain joining region blocks B-cell development and antibody production, *PNAS USA* 90:2551-2555.

Jakobovits et al., 1993, Germ-line transmission and expression of a human-derived yeast artificial chromosome, *Nature* 362:255-258.

Jang et al., 2002, Visualization of Coronary Atherosclerotic Plaques in Patients Using Optical Coherence Tomography: Comparison With Intravascular Ultrasound, *Journal of the American College of Cardiology* 39:604-609.

Jiang et al., 1992, Image registration of multimodality 3-D medical images by chamfer matching, *Proc. SPIE 1660, Biomedical Image Processing and Three-Dimensional Microscopy*, 356-366.

Johnson et al., 1993, Human antibody engineering: Current Opinion in *Structural Biology*, 3:564-571.

Jones et al., 1986, Replacing the complementarity-determining regions in a human antibody with those from a mouse, *Nature*, 321:522-525.

Juviler et al., 2008, Anorectal sepsis and fistula-in-ano, *Surgical Technology International*, 17:139-149.

Karapatis et al., 1998, Direct rapid tooling: a review of current research, *Rapid Prototyping Journal*, 4(2):77-89.

Karp et al., 2009, The benefit of time-of-flight in PET imaging, *J Nucl Med* 49:462-470.

Kelly et al., 2005, Detection of Vascular Adhesion Molecule-1 Expression Using a Novel Multimodal Nanoparticle, *Circulation Research* 96:327-336.

Kemp et al., 2005, Depth Resolved Optic Axis Orientation in Multiple Layered Anisotropic Tissues Measured with Enhanced Polarization Sensitive Optical Coherence Tomography, *Optics Express* 13(12):4507-4518.

Kersey et al., 1991, Polarization insensitive fiber optic Michelson interferometer, *Electron. Lett.* 27:518-520.

Kheir et al., 2012, Oxygen Gas-Filled Microparticles Provide Intravenous Oxygen Delivery, *Science Translational Medicine* 4(140):140ra88 (10 pages).

Khuri-Yakub et al., 2011, Capacitive micromachined ultrasonic transducers for medical imaging and therapy, *J Micromech Microeng.* 21(5):054004-054014.

Kirkman, 1991, Technique for flow reduction in dialysis access fistulas, *Surg Gyn Obstet*, 172(3):231-3.

Kohler et al., 1975, Continuous cultures of fused cells secreting antibody of predefined specificity, *Nature*, 256:495-7.

Koo et al., 2011, Diagnosis of Ischemia Causing Coronary Stenoses by Noninvasive Fractional Flow Reserve Computed From Coronary Computed Tomographic Angiograms, *J Am Coll Cardiol* 58(19):1989-1997.

Kozbor et al., 1984, A human hybrid myeloma for production of human monoclonal antibodies, *J. Immunol.*, 133:3001-3005.

Kruth et al., 2003, Lasers and materials in selective laser sintering, *Assembly Automation*, 23(4):357-371.

Kumagai et al., 1994, Ablation of polymer films by a femtosecond high-peak-power Ti:sapphire laser at 798 nm, *Applied Physics Letters*, 65(14):1850-1852.

(56)

References Cited

OTHER PUBLICATIONS

- Larin et al., 2002, Noninvasive Blood Glucose Monitoring with Optical Coherence Tomography: a pilot study in human subjects, *Diabetes Care*, 25(12):2263-7.
- Larin et al., 2004, Measurement of Refractive Index Variation of Physiological Analytes using Differential Phase OCT, *Proc of SPIE* 5325:31-34.
- Laufer, 1996, *Introduction to Optics and Lasers in Engineering*, Cambridge University Press, Cambridge UK:156-162.
- Lefevre et al., 2001, Stenting of bifurcation lesions: a rational approach, *J. Interv. Cardiol.*, 14(6):573-585.
- Li et al., 2000, Optical Coherence Tomography: Advanced Technology for the Endoscopic Imaging of Barrett's Esophagus, *Endoscopy*, 32(12):921-930.
- Abdi et al., 2010, Principal component analysis, *Wiley Interdisciplinary Reviews: Computational Statistics* 2:433-459.
- Adler et al., 2007, Phase-Sensitive Optical Coherence Tomography at up to 370,000 Lines Per Second Using Buffered Fourier Domain Mode-Locked Lasers, *Optics Letters*, 32(6):626-628.
- Agresti, 1996, Models for Matched Pairs, Chapter 8, *An Introduction to Categorical Data Analysis*, Wiley-Interscience A John Wiley & Sons, Inc., Publication, Hoboken, New Jersey.
- Akashah et al., 2004, Development of piezoelectric micromachined ultrasonic transducers, *Sensors and Actuators A Physical*, 111:275-287.
- Amini et al., 1990, Using dynamic programming for solving variational problems in vision, *IEEE Transactions on Pattern Analysis and Machine Intelligence*, 12(9):855-867.
- Bail et al., 1996, Optical coherence tomography with the "Spectral Radar"—Fast optical analysis in volume scatterers by short coherence interferometry, *Optics Letters* 21(14):1087-1089.
- Bain, 2011, Privacy protection and face recognition, Chapter 3, *Handbook of Face Recognition*, Stan et al., Springer-Verlag.
- Barnea et al., 1972, A class of algorithms for fast digital image registration, *IEEE Trans. Computers*, 21(2):179-186.
- Blanchet et al., 1993, Laser Ablation and the Production of Polymer Films, *Science*, 262(5134):719-721.
- Bonnema, 2008, *Imaging Tissue Engineered Blood Vessel Mimics with Optical Tomography*, College of Optical Sciences dissertation, University of Arizona (252 pages).
- Bouma et al., 1999, Power-efficient nonreciprocal interferometer and linear-scanning fiber-optic catheter for optical coherence tomography, *Optics Letters*, 24(8):531-533.
- Breiman, 2001, Random forests, *Machine Learning* 45:5-32.
- Brown, 1992, A survey of image registration techniques, *ACM Computing Surveys* 24(4):325-376.
- Bruining et al., 2009, Intravascular Ultrasound Registration/Integration with Coronary Angiography, *Cardiology Clinics*, 27(3):531-540.
- Brummer, 1997, An euclidean distance measure between covariance matrices of speech spectra for text-independent speaker recognition, in *Proc. South African Symp. Communications and Signal Processing*:167-172.
- Burr et al., 2005, Searching for the Center of an Ellipse in Proceedings of the 17th Canadian Conference on Computational Geometry:260-263.
- Canny, 1986, A computational approach to edge detection, *IEEE Trans. Pattern Anal. Mach. Intell.* 8:679-698.
- Cavalli et al., 2010, Nanosponge formulations as oxygen delivery systems, *International Journal of Pharmaceutics* 402:254-257.
- Choma et al., 2003, Sensitivity Advantage of Swept Source and Fourier Domain Optical Coherence Tomography, *Optics Express* 11(18):2183-2189.
- Clarke et al., 1995, Hypoxia and myocardial ischaemia during peripheral angioplasty, *Clinical Radiology*, 50(5):301-303.
- Collins, 1993, Coronary flow reserve, *British Heart Journal* 69:279-281.
- Communication Mechanisms for Distributed Real-Time Applications, NI Developer Zone, <http://zone.ni.com/devzone/cda/tut/p/id/3105>, accessed Jul. 23, 2007.
- Cook, 2007, Use and misuse of receiver operating characteristic curve in risk prediction, *Circulation* 115(7):928-35.
- D'Agostino et al., 2001, Validation of the Framingham coronary heart disease prediction score: results of a multiple ethnic group investigation, *JAMA* 286:180-187.
- David et al., 1974, Protein iodination with solid-state lactoperoxidase, *Biochemistry* 13:1014-1021.
- Davies et al., 1985, Plaque fissuring—the cause of acute myocardial infarction, sudden ischaemic death, and crescendo angina, *British Heart Journal* 53:363-373.
- Davies et al., 1993, Risk of thrombosis in human atherosclerotic plaques: role of extracellular lipid, macrophage, and smooth muscle cell content, *British Heart Journal* 69:377-381.
- Deterministic Data Streaming in Distributed Data Acquisition Systems, NI Developer Zone, "What is Developer Zone?", <http://zone.ni.com/devzone/cda/tut/p/id/3105>, accessed Jul. 23, 2007.
- Eigenwillig, 2008, K-Space Linear Fourier Domain Mode Locked Laser and Applications for Optical Coherence Tomography, *Optics Express* 16(12):8916-8937.
- Elghanian et al., 1997, Selective colorimetric detection of polynucleotides based on the distance-dependent optical properties of gold nanoparticles, *Science*, 277(5329):1078-1080.
- Ergun et al., 2003, Capacitive Micromachined Ultrasonic Transducers: Theory and Technology, *Journal of Aerospace Engineering*, 16(2):76-84.
- Evans et al., 2006, Optical coherence tomography to identify intramucosa carcinoma and high-grade dysplasia in Barrett's esophagus, *Clin Gast Hepat* 4(1):38-43.
- Fatemi et al., 1999, Vibro-acoustography: an imaging modality based on ultrasound-stimulated acoustic emission, *PNAS U.S.A.*, 96(12):6603-6608.
- Felzenszwalb et al., 2005, Pictorial Structures for Object Recognition, *International Journal of Computer Vision*, 61(1):55-79.
- Ferring et al., 2008, Vasculature ultrasound for the pre-operative evaluation prior to arteriovenous fistula formation for haemodialysis: review of the evidence, *Nephrol. Dial. Transplant.* 23(6):1809-1815.
- Fischler et al., 1973, The representation and matching of pictorial structures, *IEEE Transactions on Computer* 22:67-92.
- Fleming et al., 2010, Real-time monitoring of cardiac radio-frequency ablation lesion formation using an optical coherence tomography forward-imaging catheter, *Journal of Biomedical Optics* 15 (3):030516-1 (3 pages).
- Fookes et al., 2002, Rigid and non-rigid image registration and its association with mutual information: A review, Technical Report ISBN:1 86435 569 7, RCCVA, QUT.
- Forstner & Moonen, 1999, A metric for covariance matrices, In Technical Report of the Dpt of Geodesy and Geoinformatics, Stuttgart University, 113-128.
- Goel et al., 2006, Minimally Invasive Limited Ligation Endoluminal-assisted Revision (Miller) for treatment of dialysis access-associated steal syndrome, *Kidney Int* 70(4):765-70.
- Gotzinger et al., 2005, High speed spectral domain polarization sensitive optical coherence tomography of the human retina, *Optics Express* 13(25):10217-10229.
- Gould et al., 1974, Physiologic basis for assessing critical coronary stenosis, *American Journal of Cardiology*, 33:87-94.
- Griffiths et al., 1993, Human anti-self antibodies with high specificity from phage display libraries, *The EMBO Journal*, 12:725-734.
- Griffiths et al., 1994, Isolation of high affinity human antibodies directly from large synthetic repertoires, *The EMBO Journal*, 13(14):3245-3260.
- Grund et al., 2010, Analysis of biomarker data: logs, odds, ratios and ROC curves, *Curr Opin HIV AIDS* 5(6):473-479.
- Harrison et al., 2011, Guidewire Stiffness: What's in a name?, *J Endovasc Ther*, 18(6):797-801.
- Huber et al., 2005, Amplified, Frequency Swept Lasers for Frequency Domain Reflectometry and OCT Imaging: Design and Scaling Principles, *Optics Express* 13(9):3513-3528.
- Huber et al., 2006, Fourier Domain Mode Locking (FDML): A New Laser Operating Regime and Applications for Optical Coherence Tomography, *Optics Express* 14(8):3225-3237.

(56)

References Cited

OTHER PUBLICATIONS

International Search Report and Written Opinion dated Mar. 11, 2014, for International Patent Application No. PCT/US13/75675, filed Dec. 17, 2013 (7 pages).

International Search Report and Written Opinion dated Mar. 19, 2014, for International Patent Application No. PCT/US13/075353, filed Dec. 16, 2013 (8 pages).

* cited by examiner

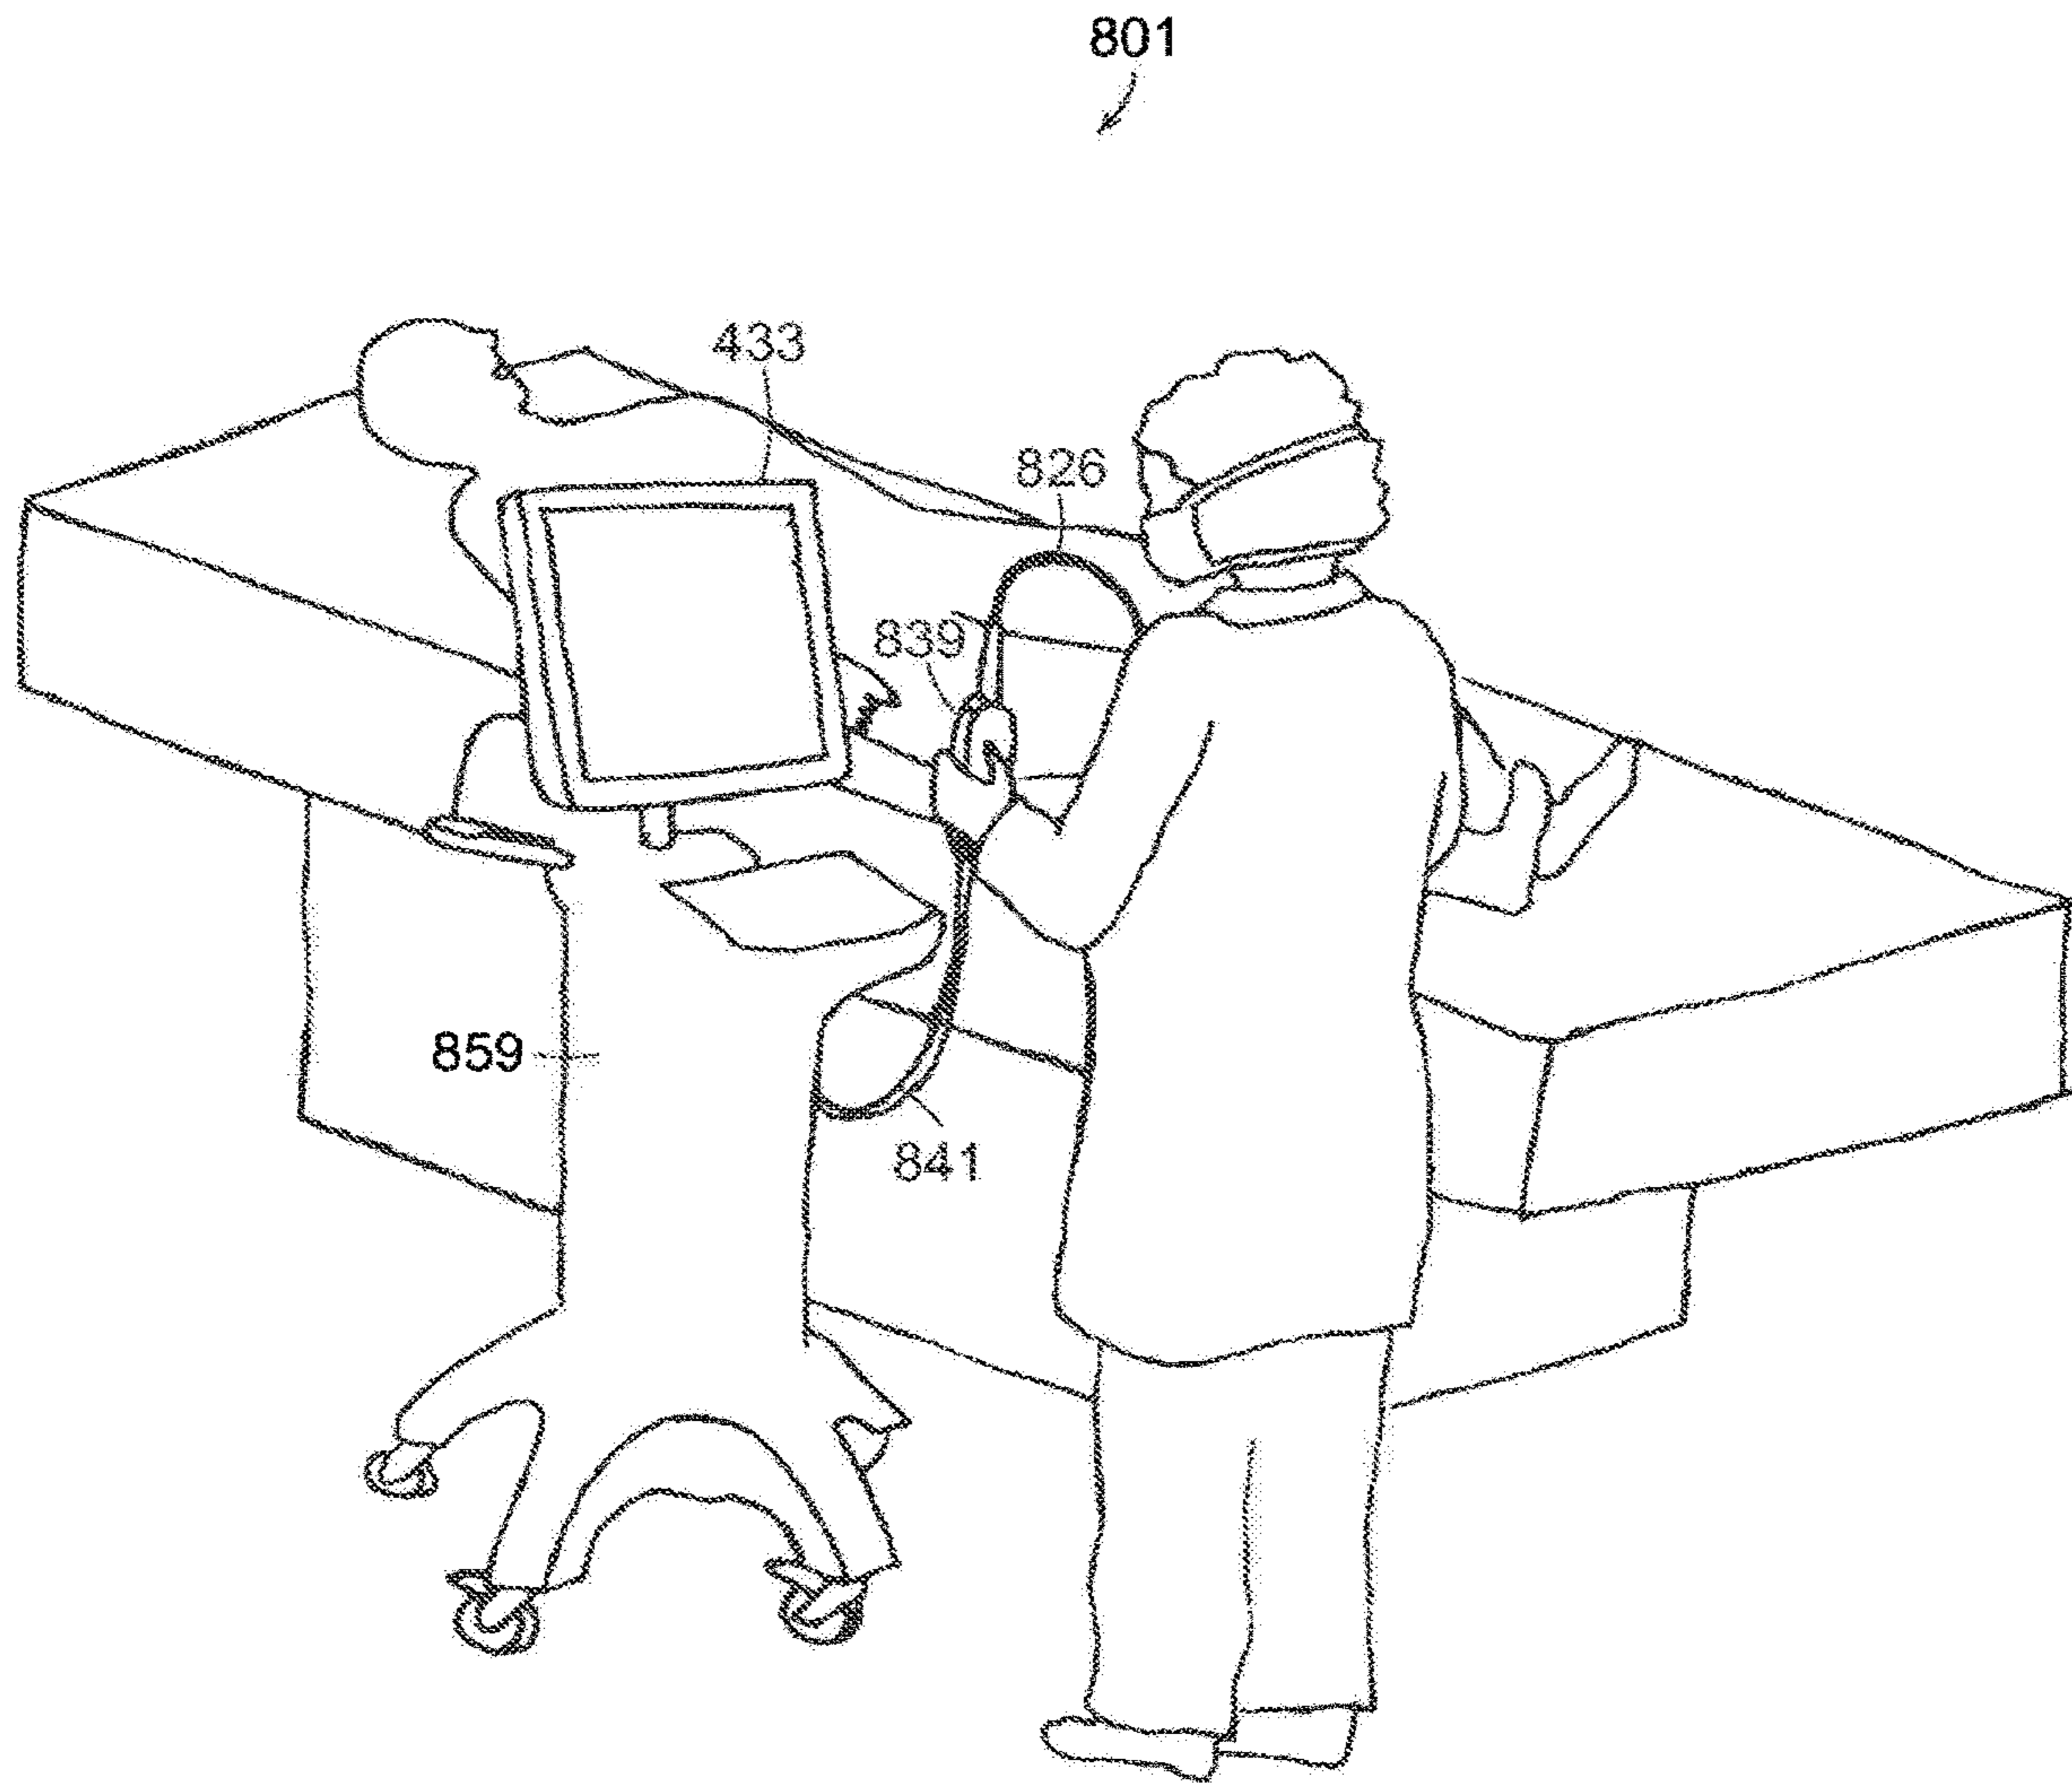


FIG. 1

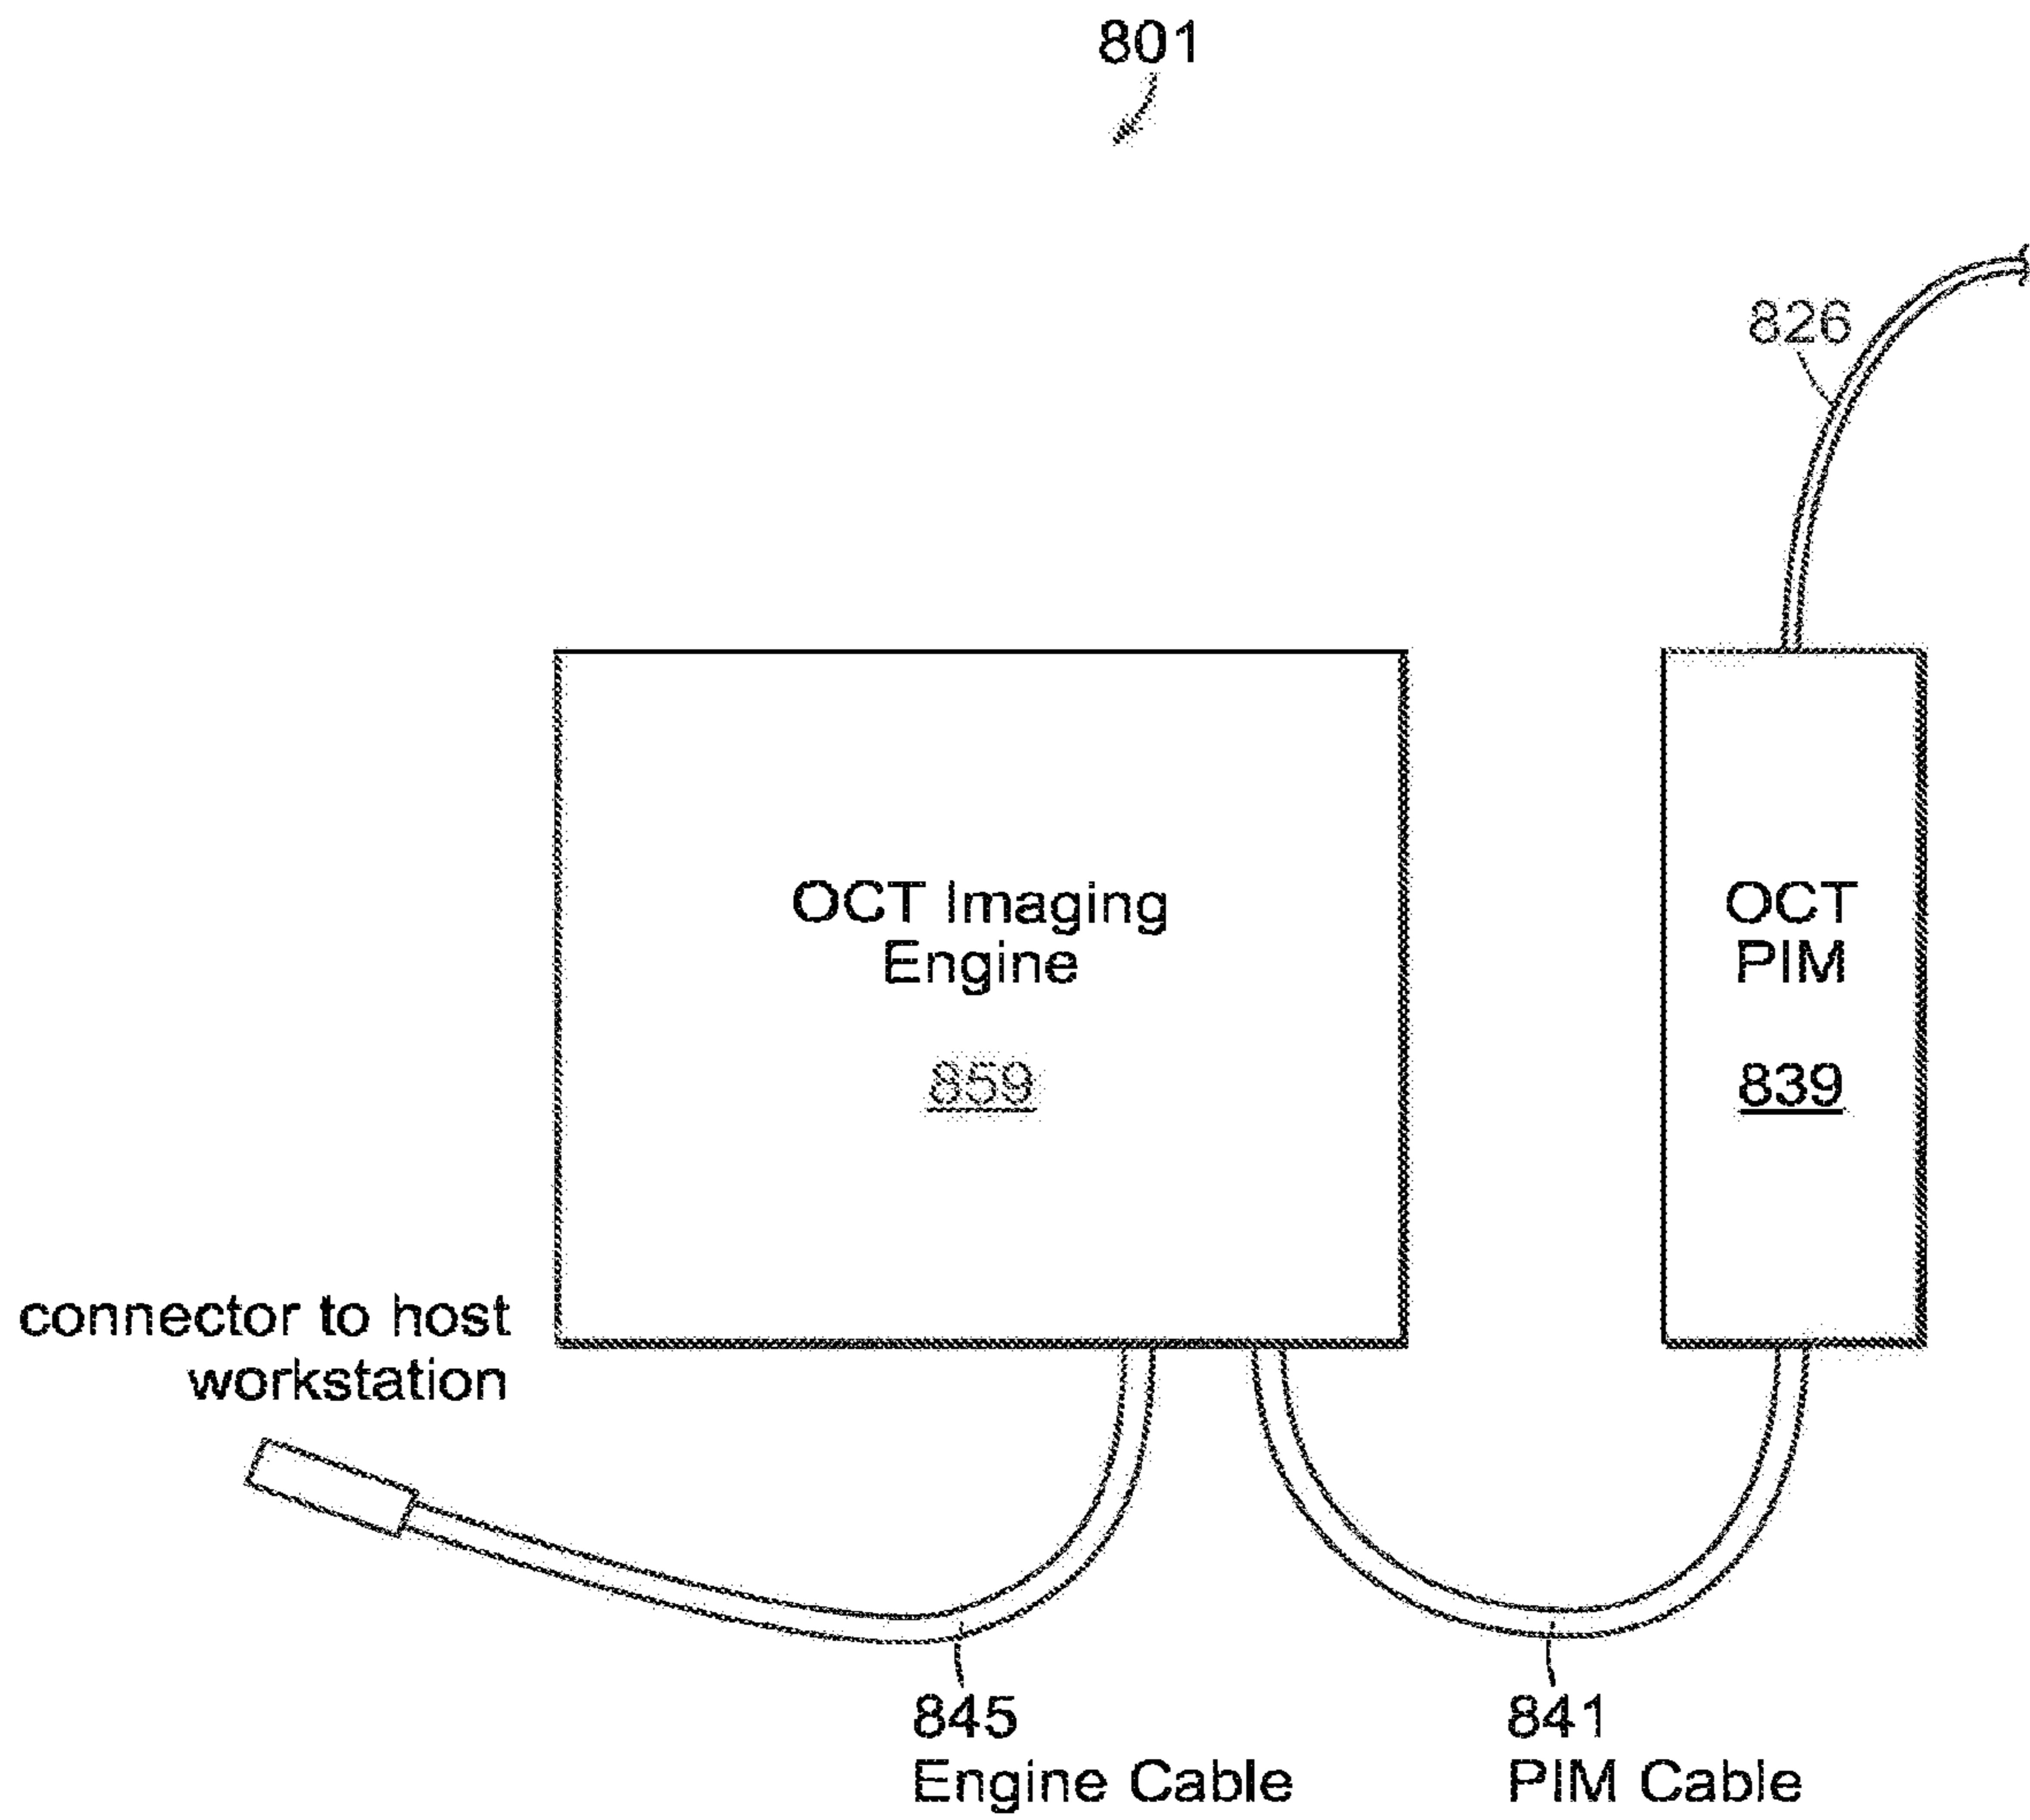


FIG. 2

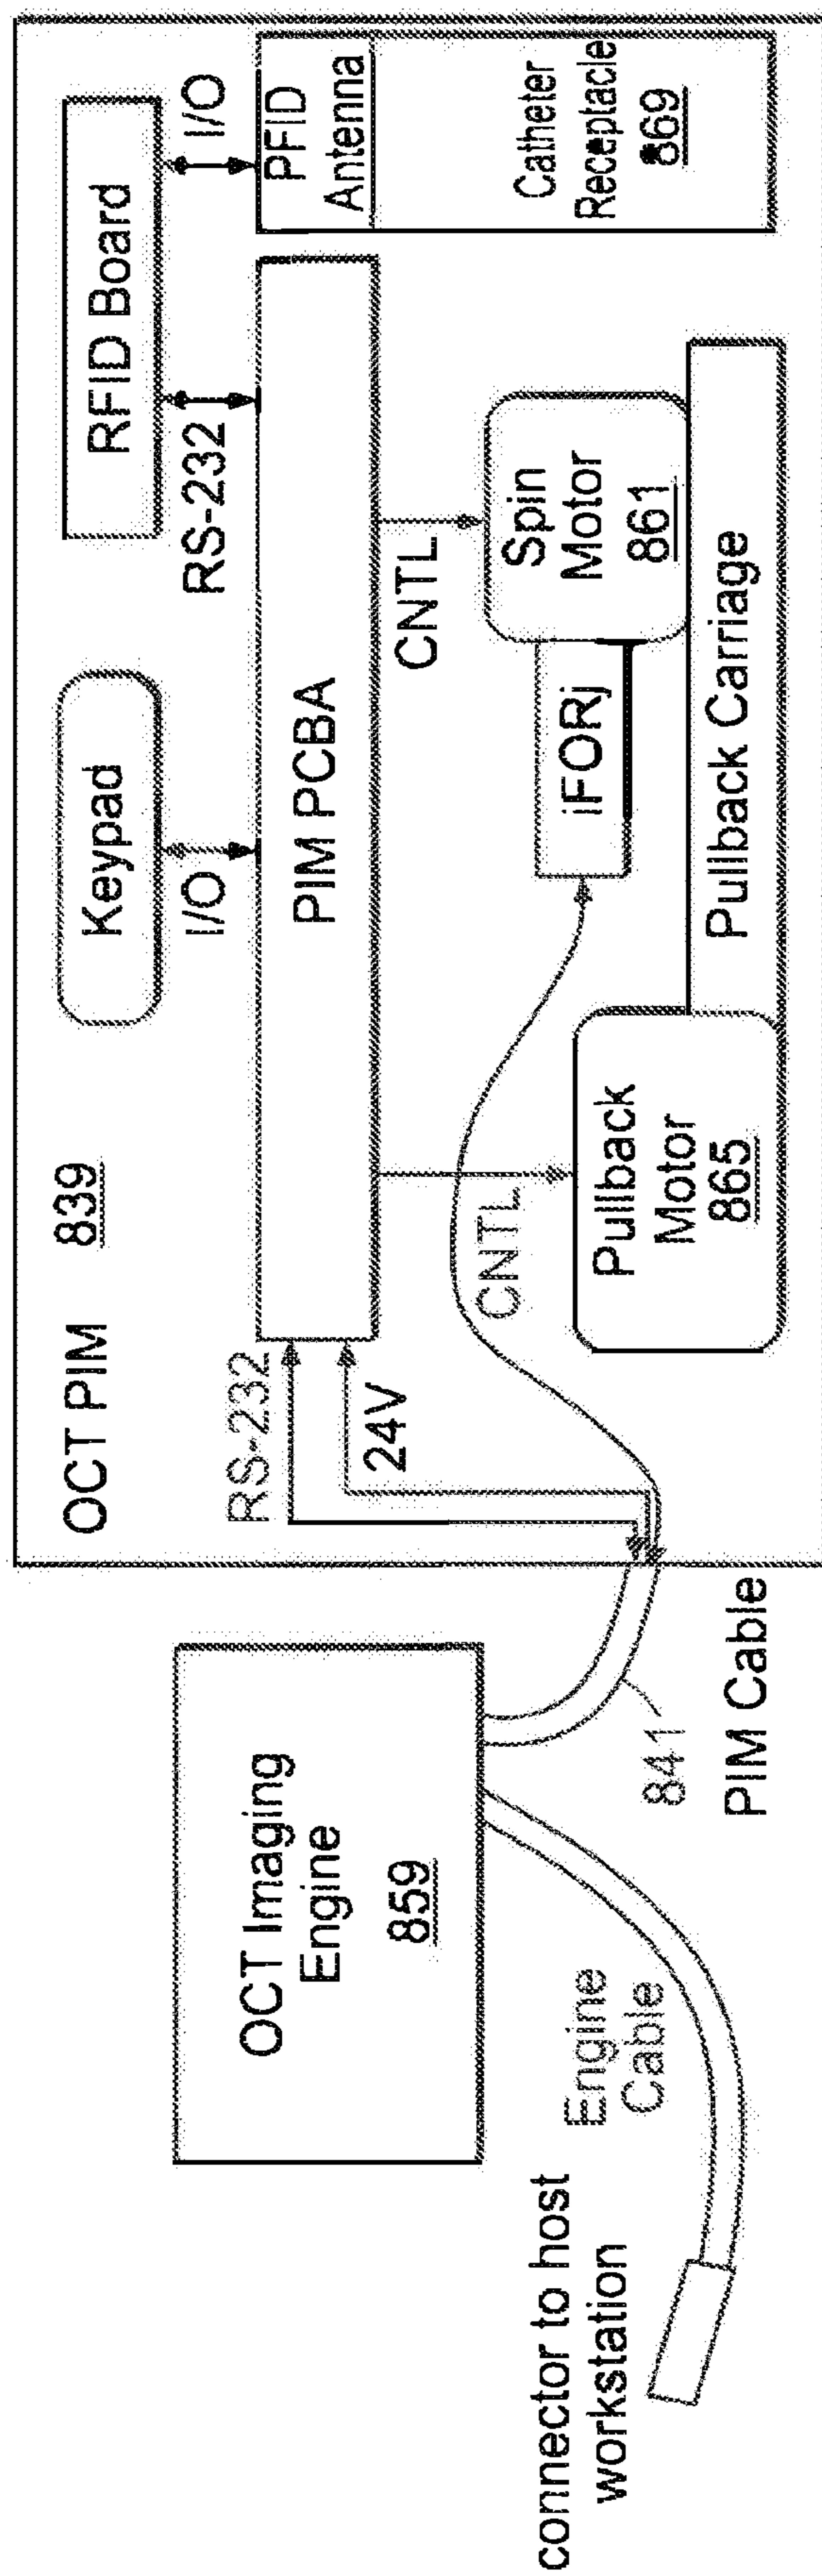


FIG. 3

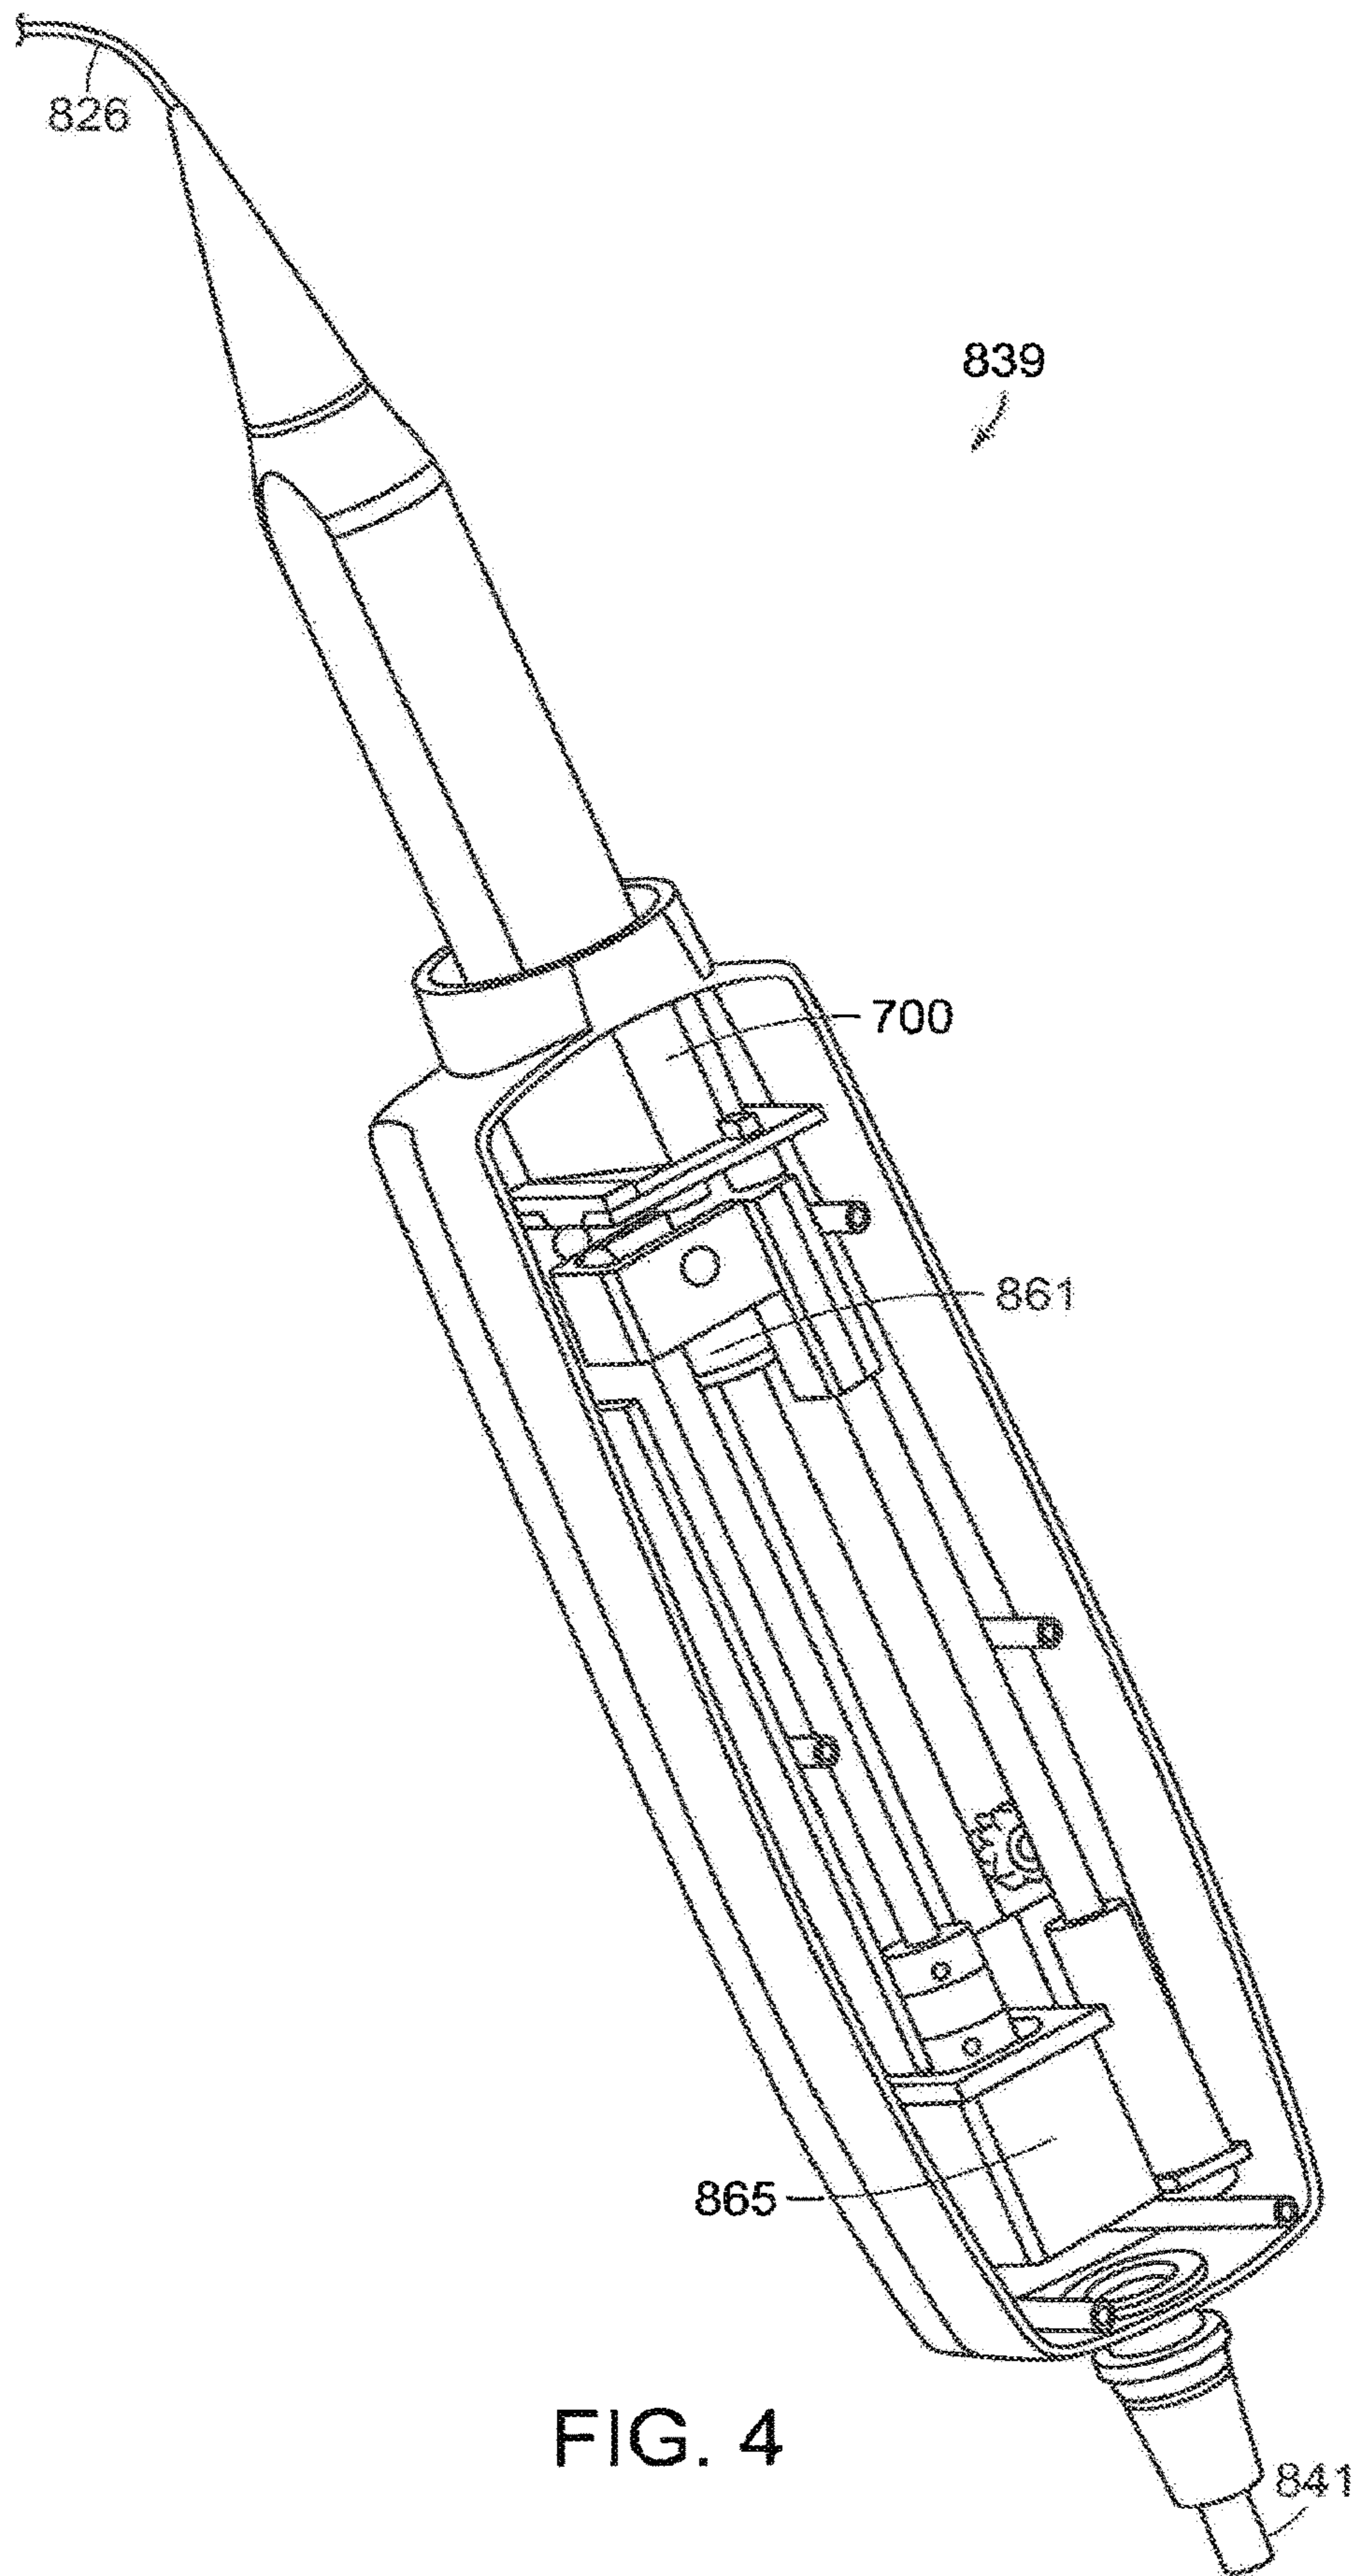


FIG. 4

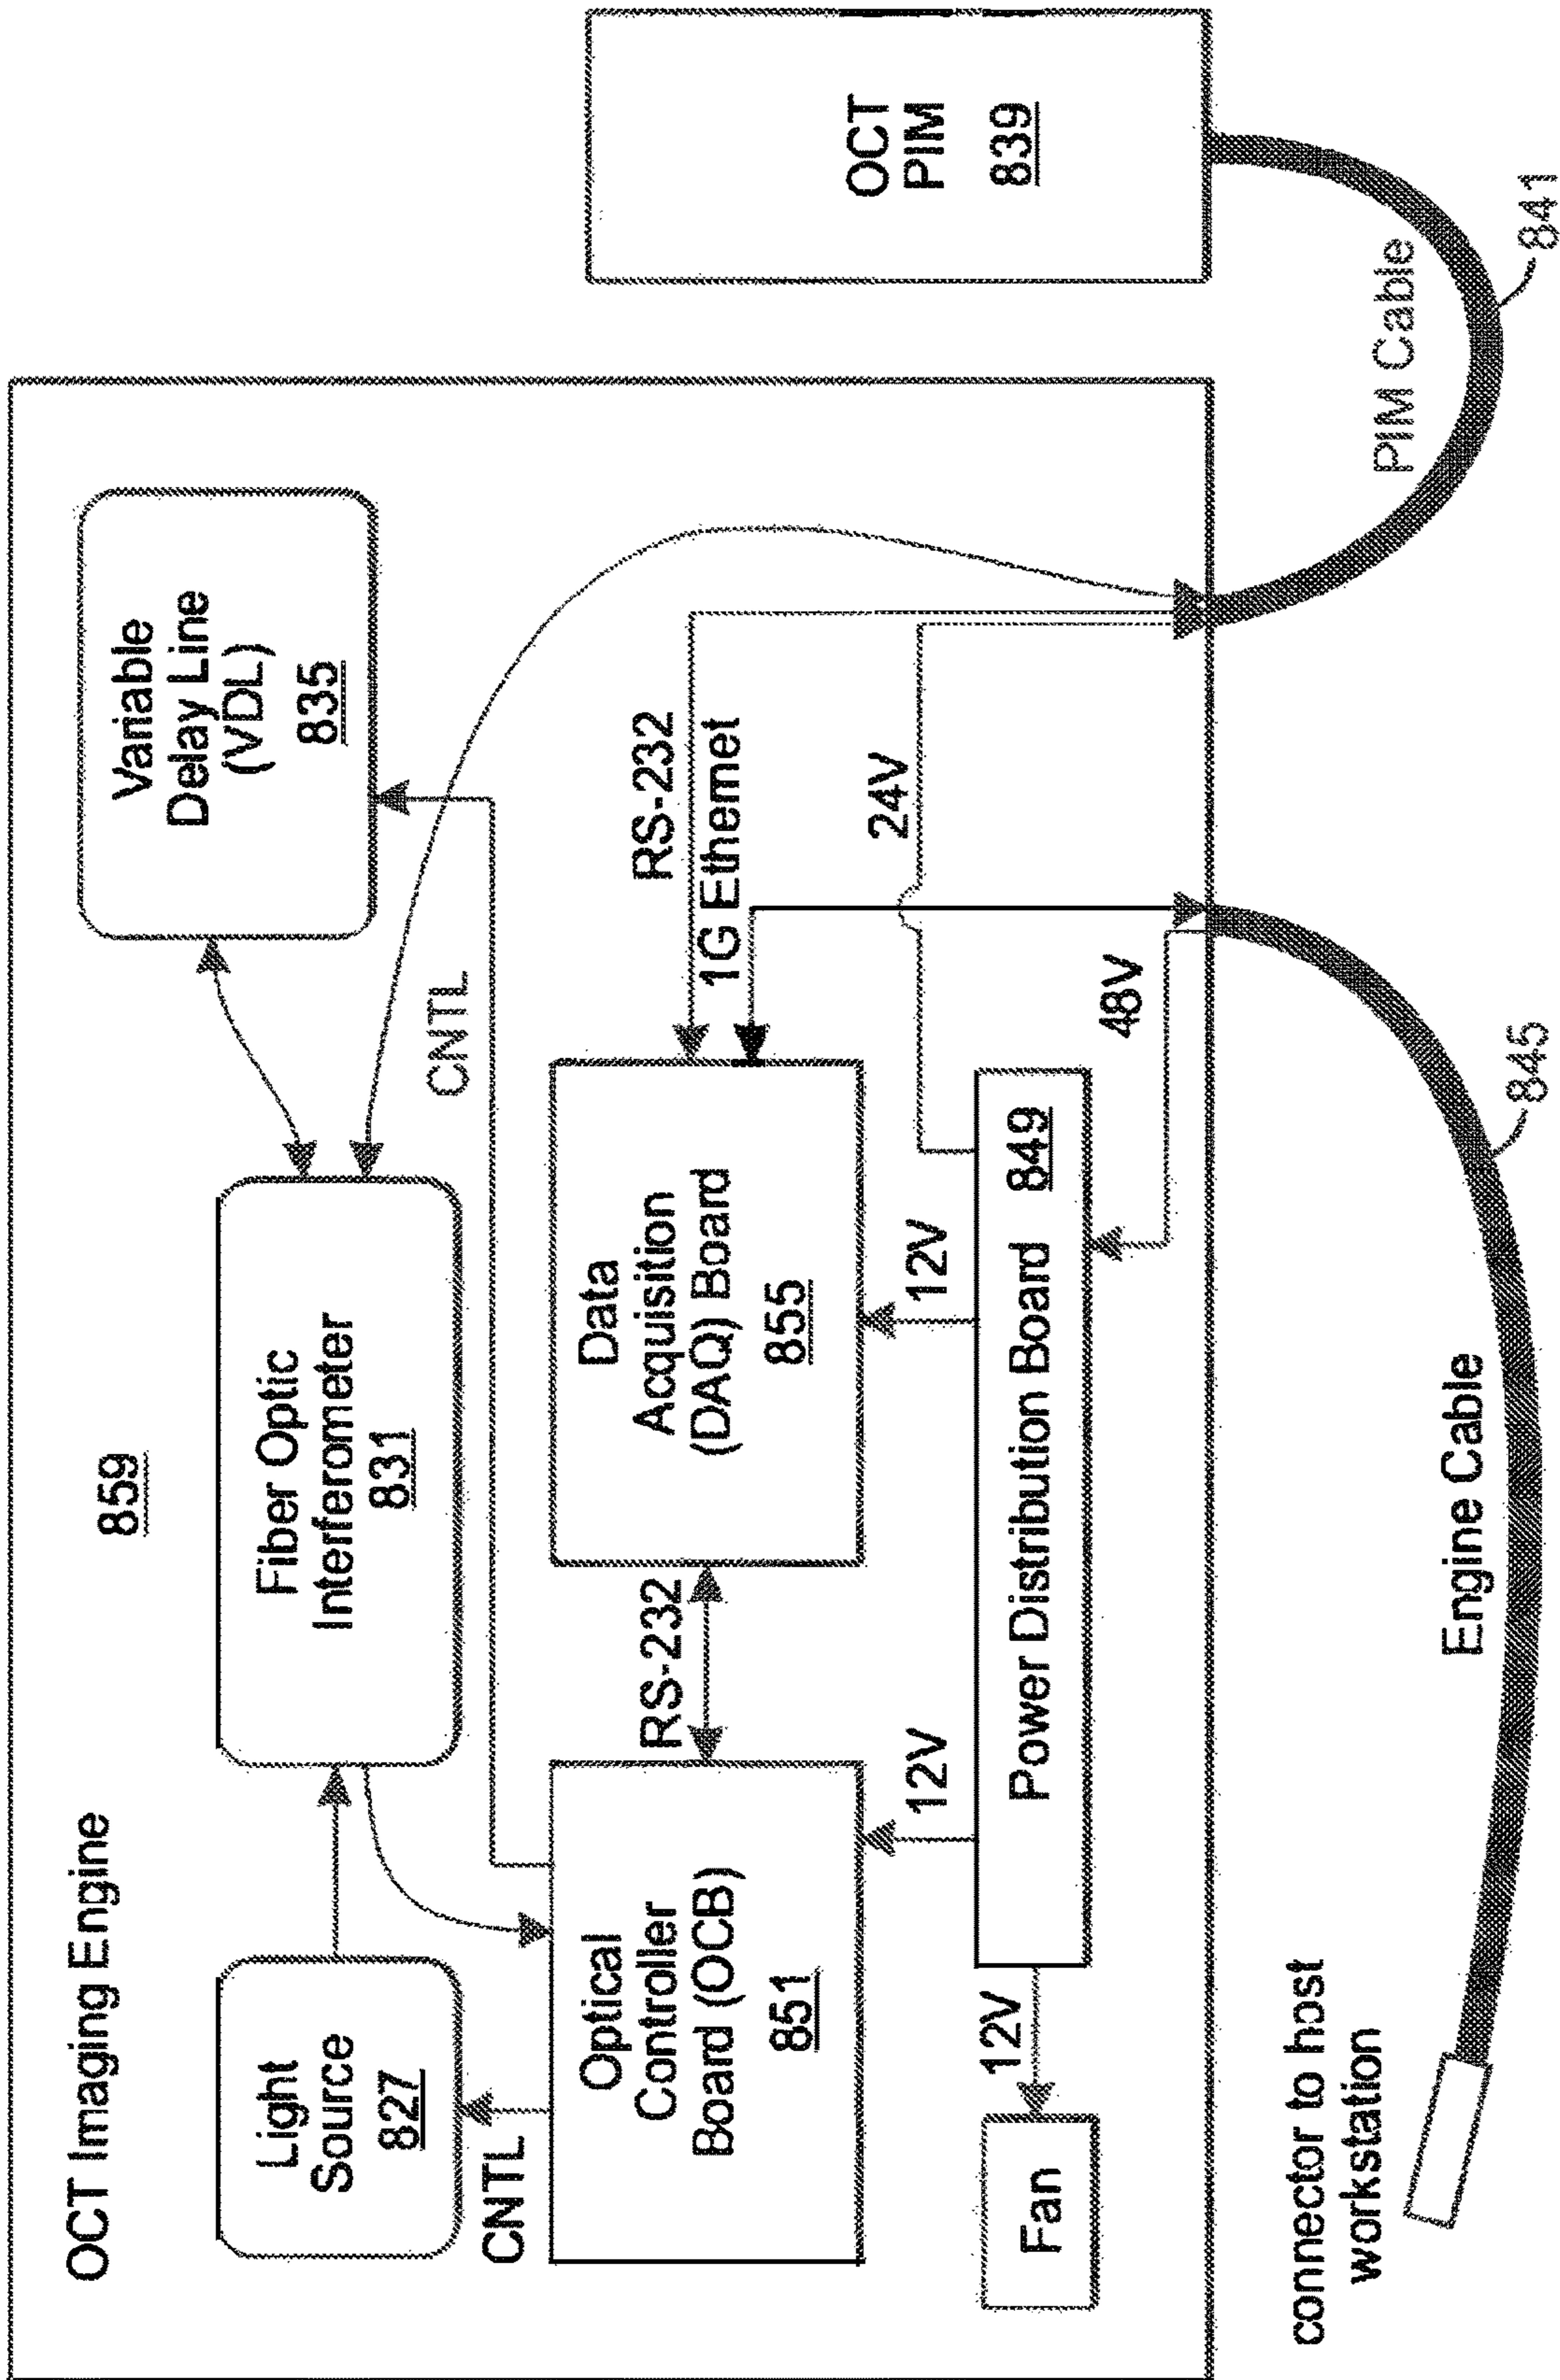


FIG. 5

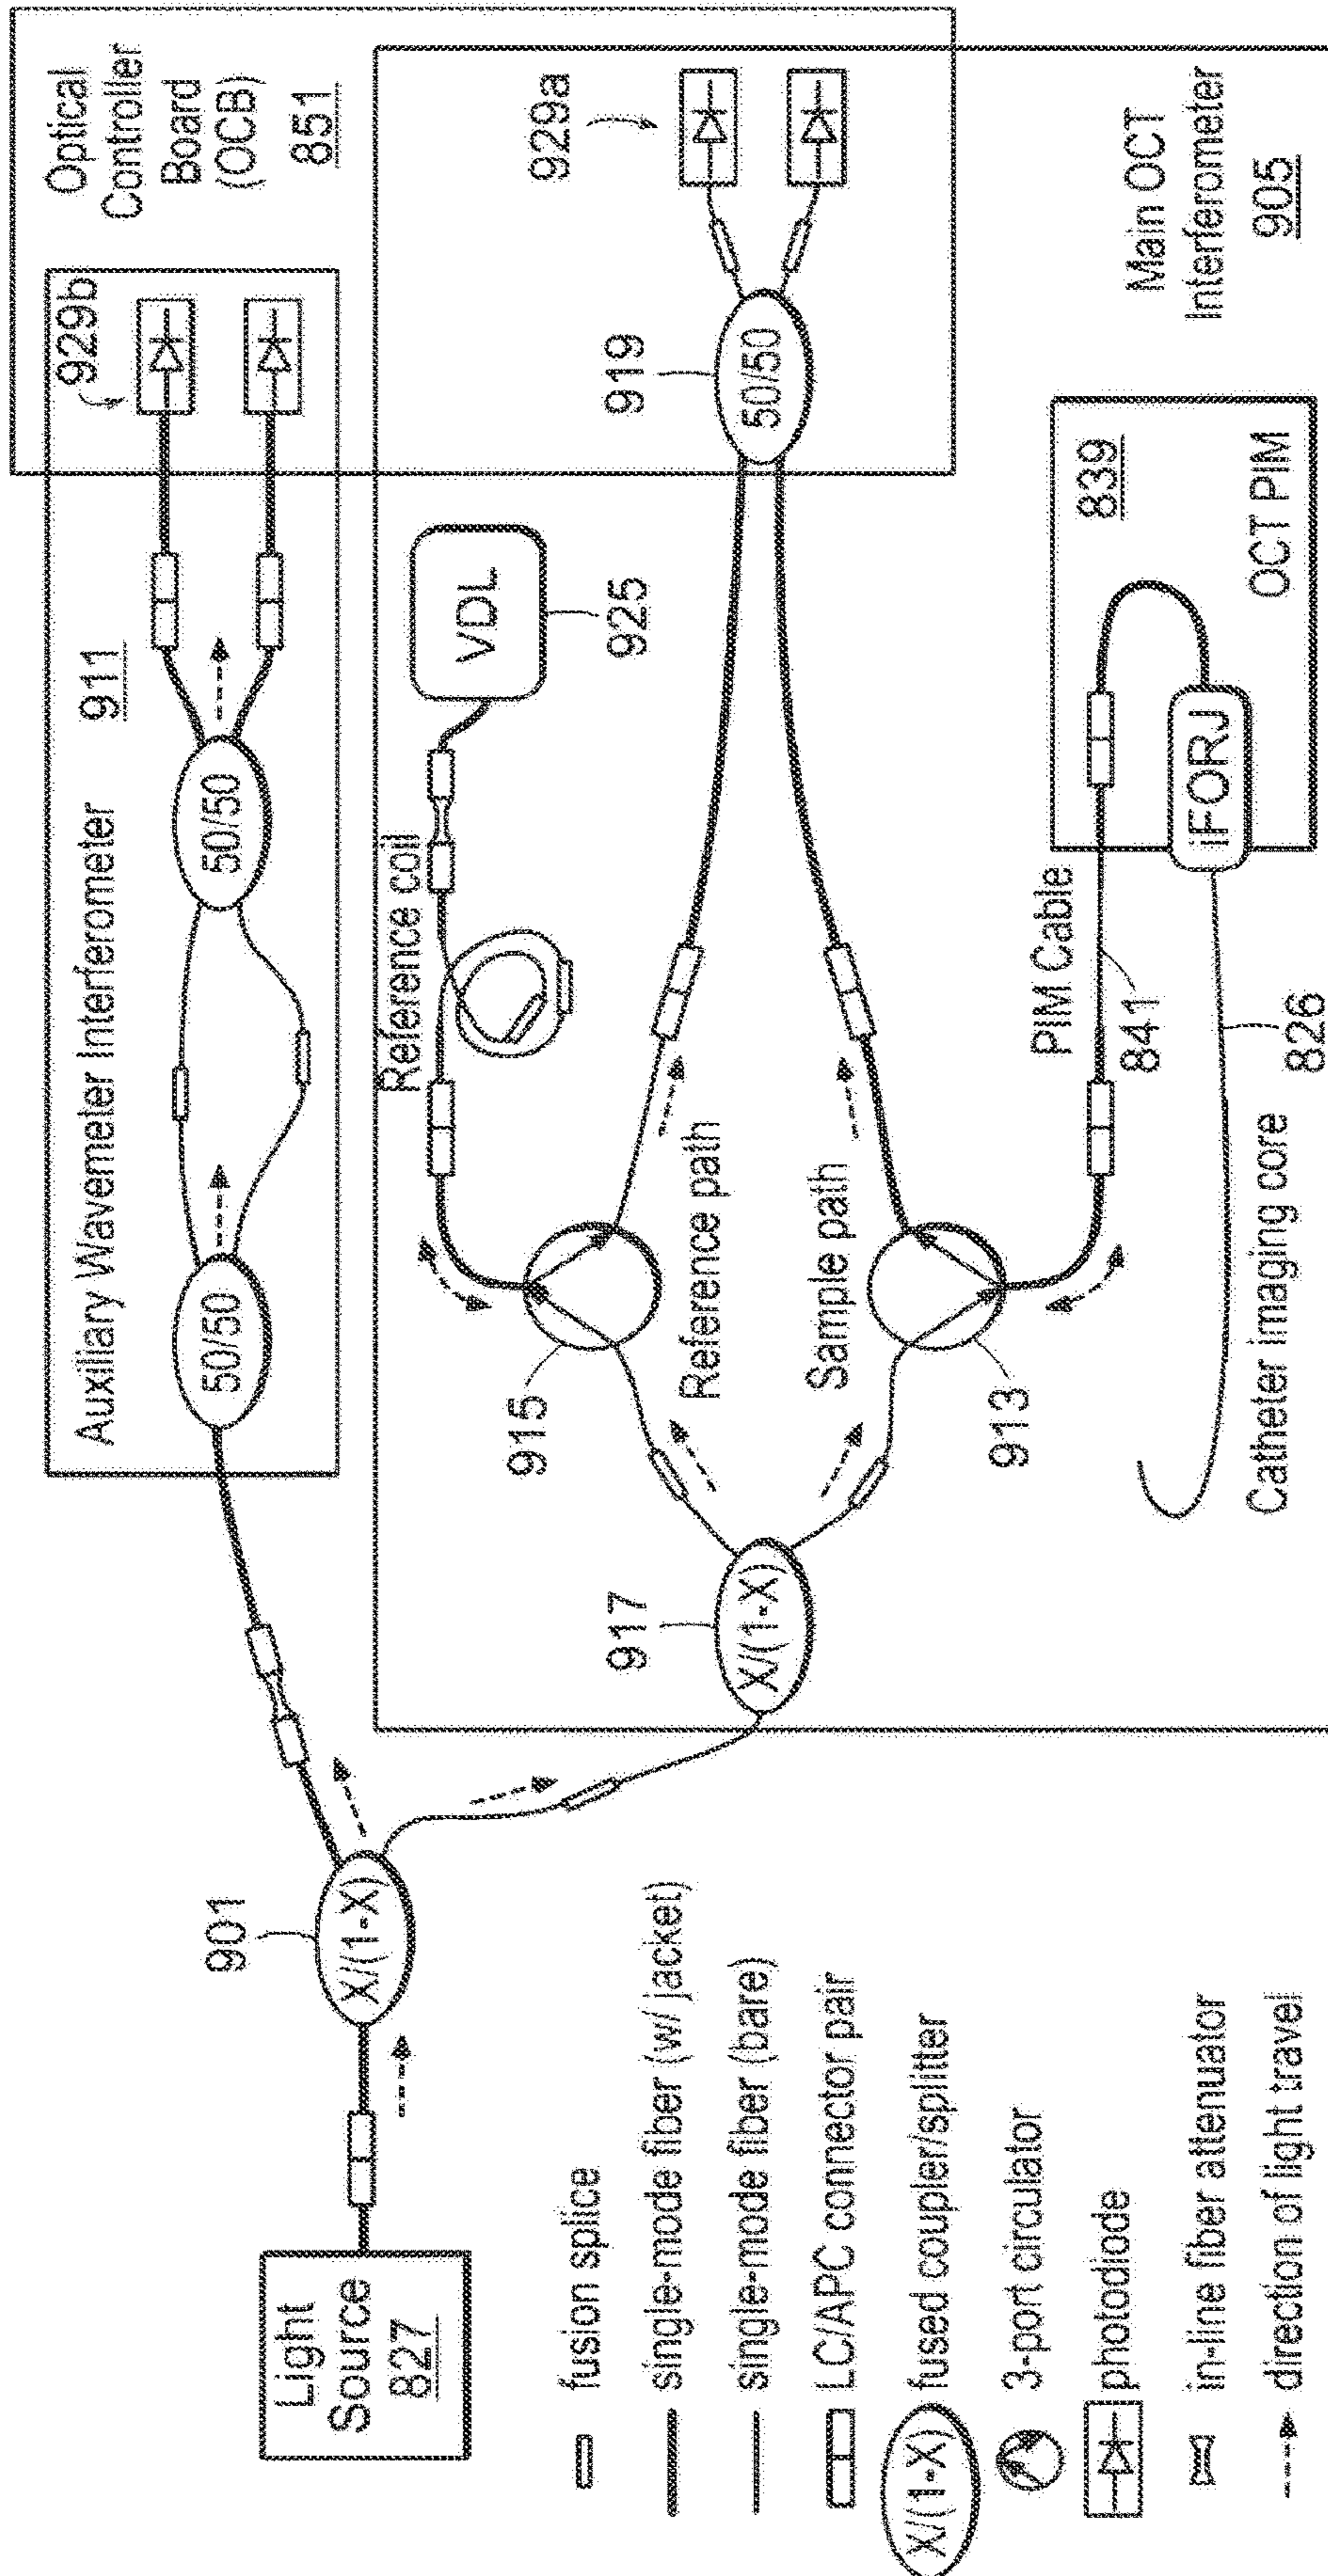


FIG. 6

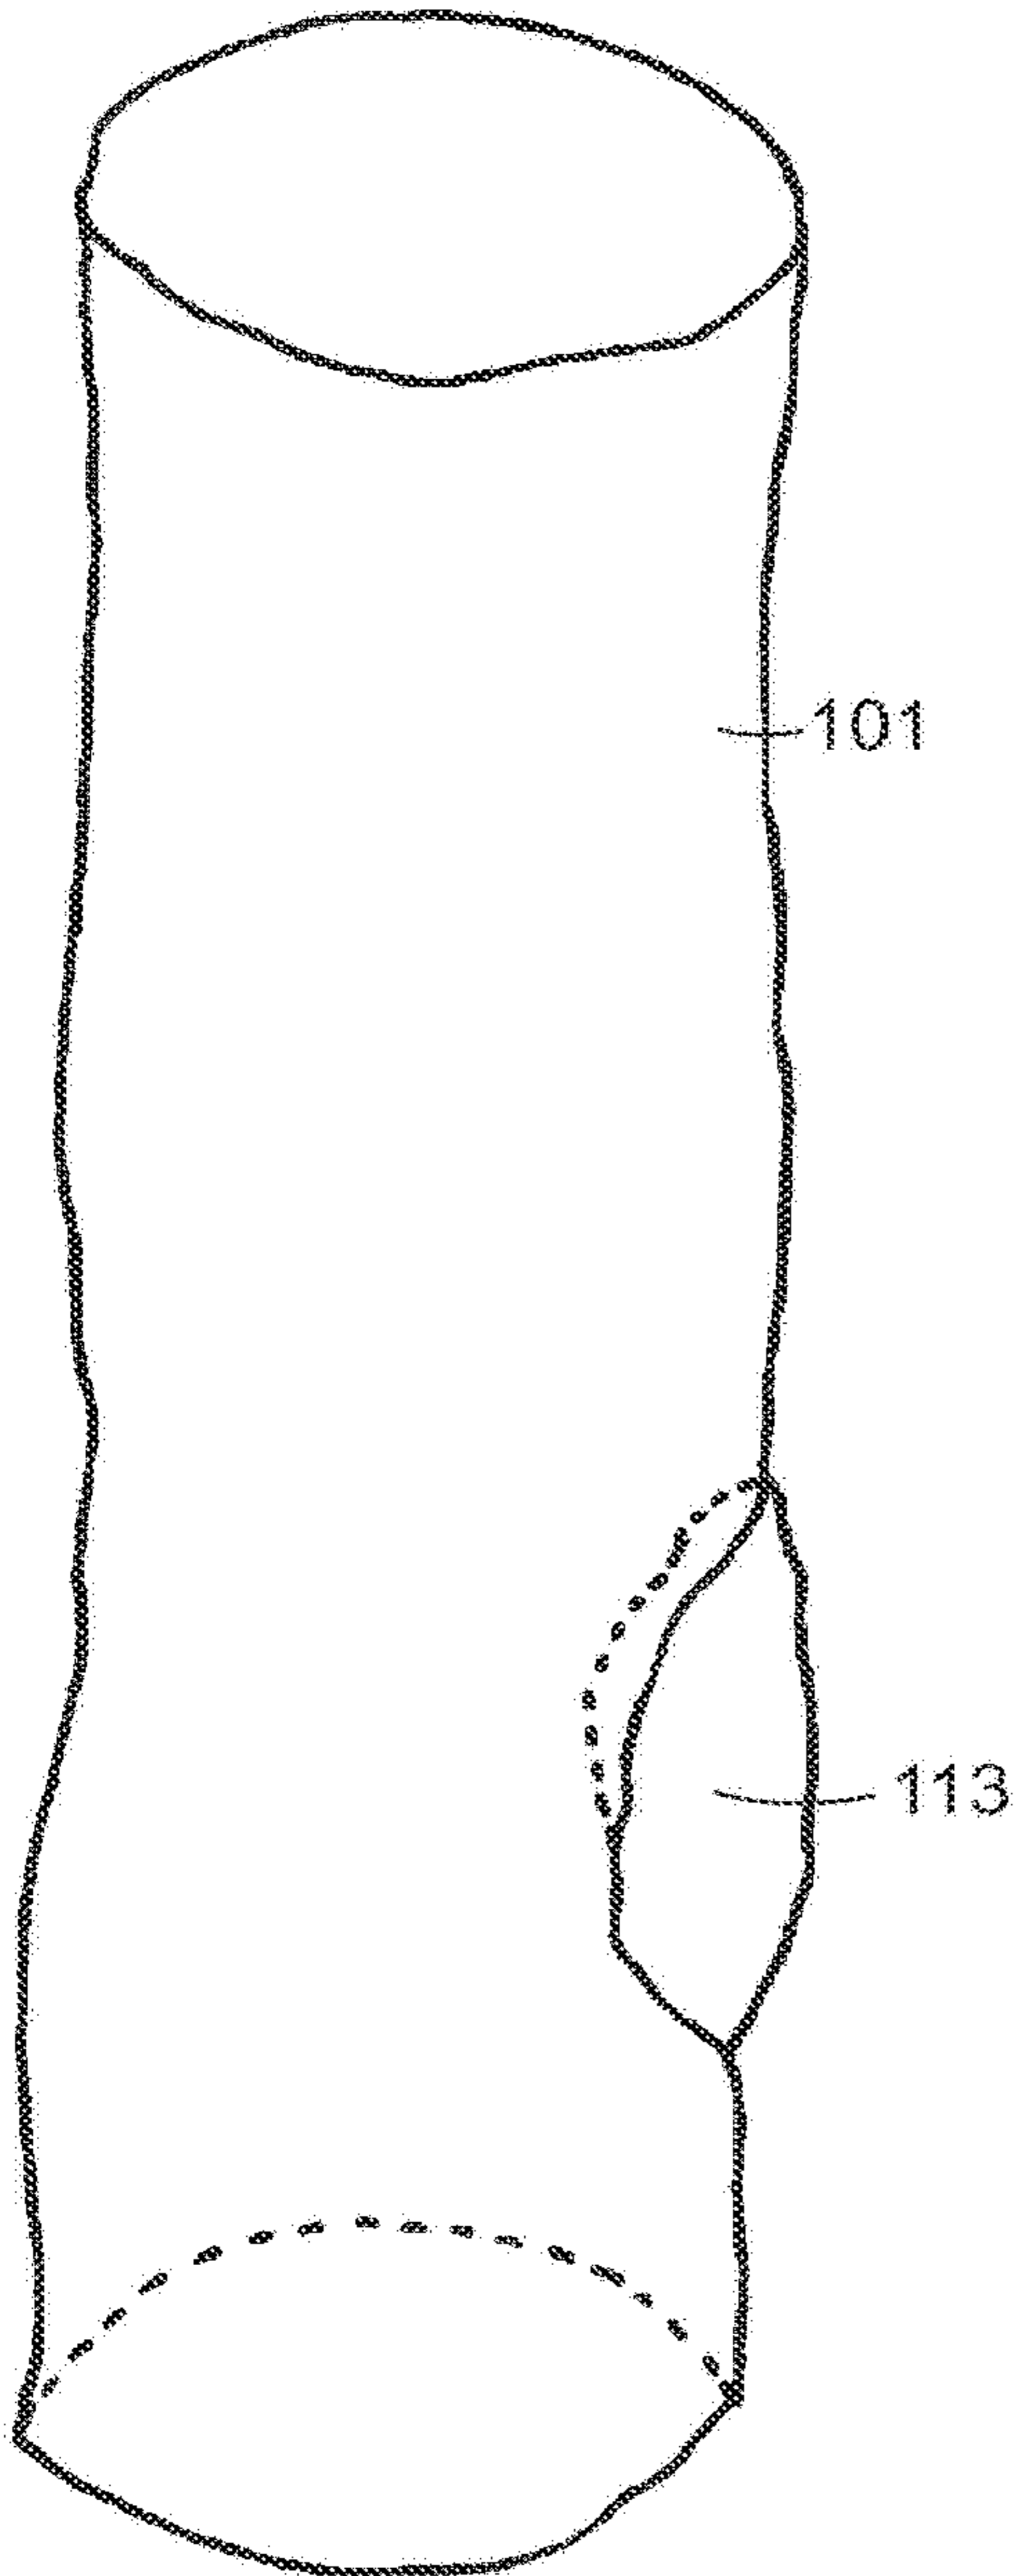


FIG. 7A

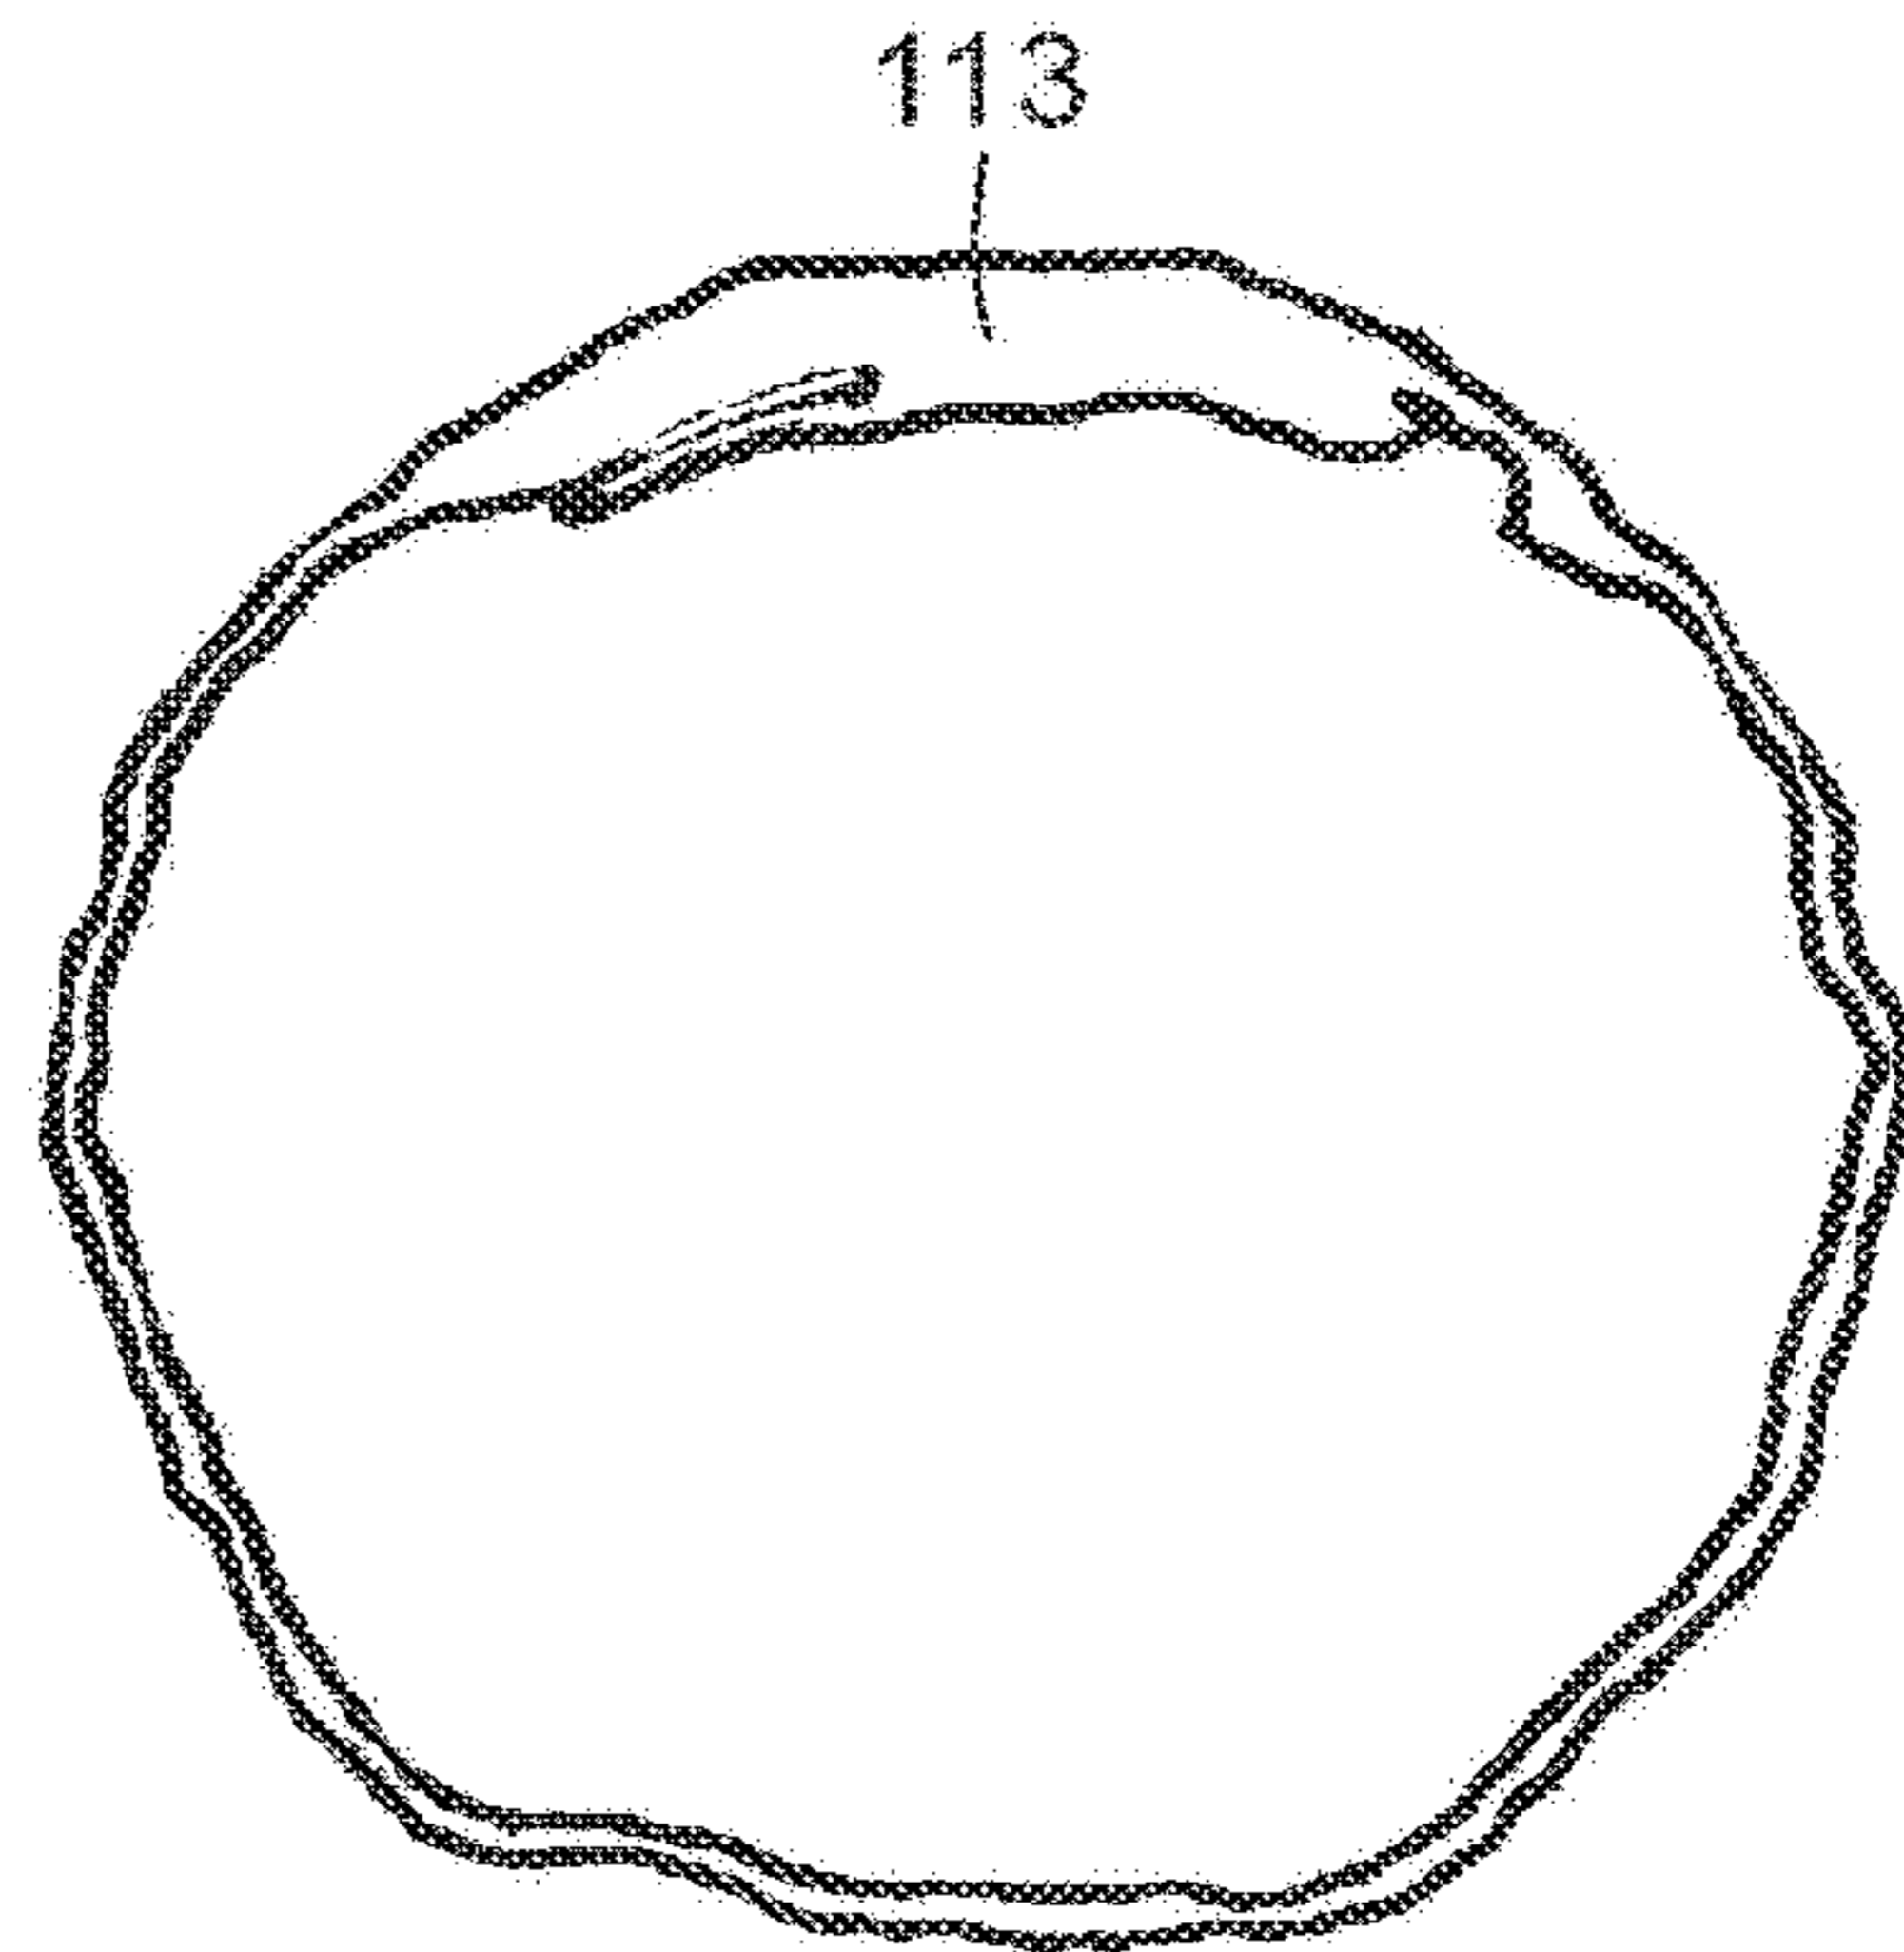


FIG. 7B

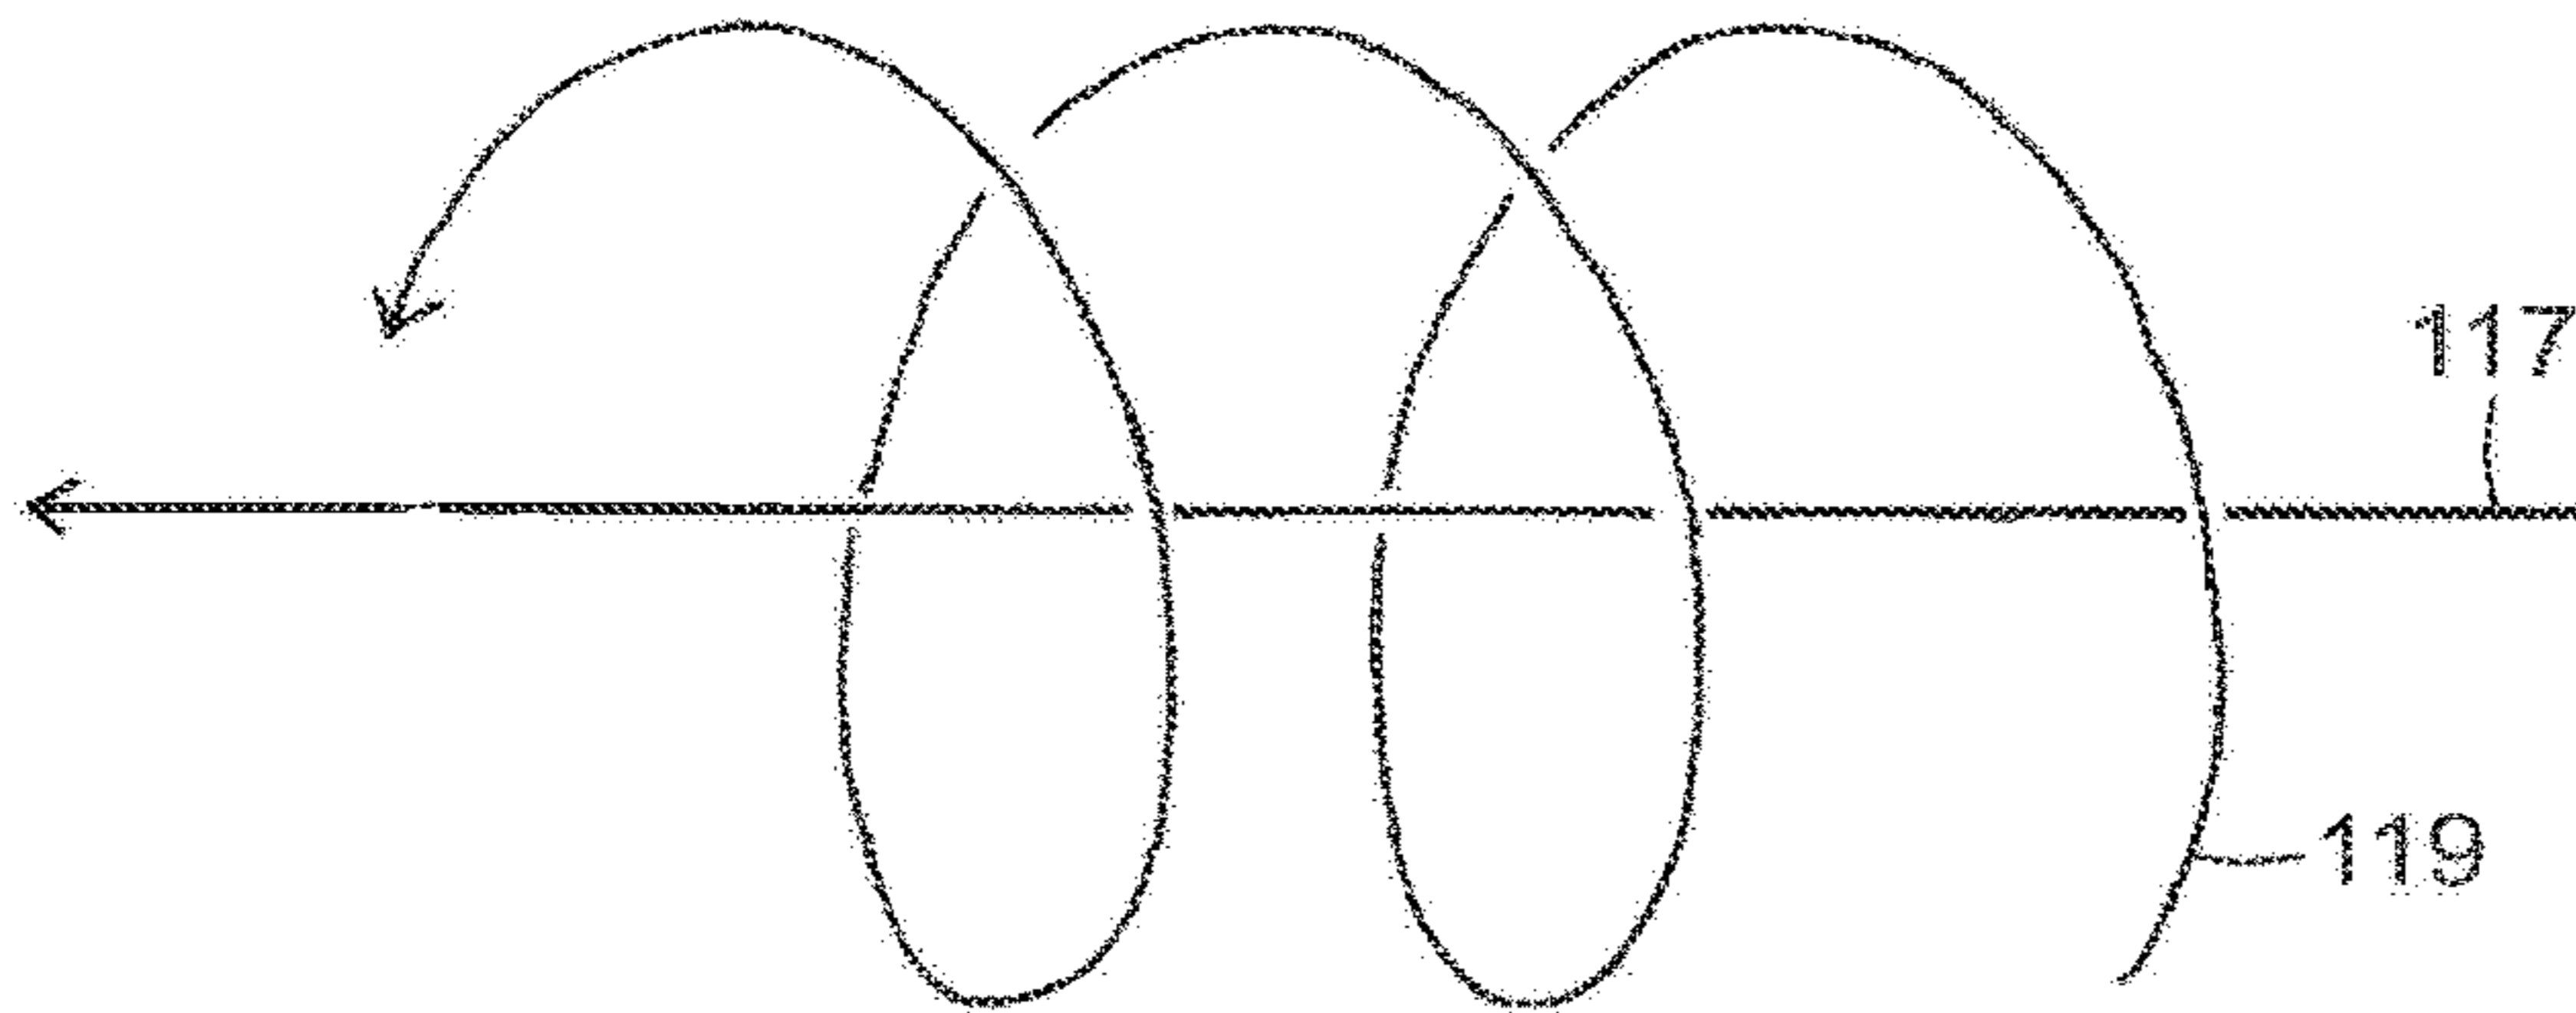


FIG. 8

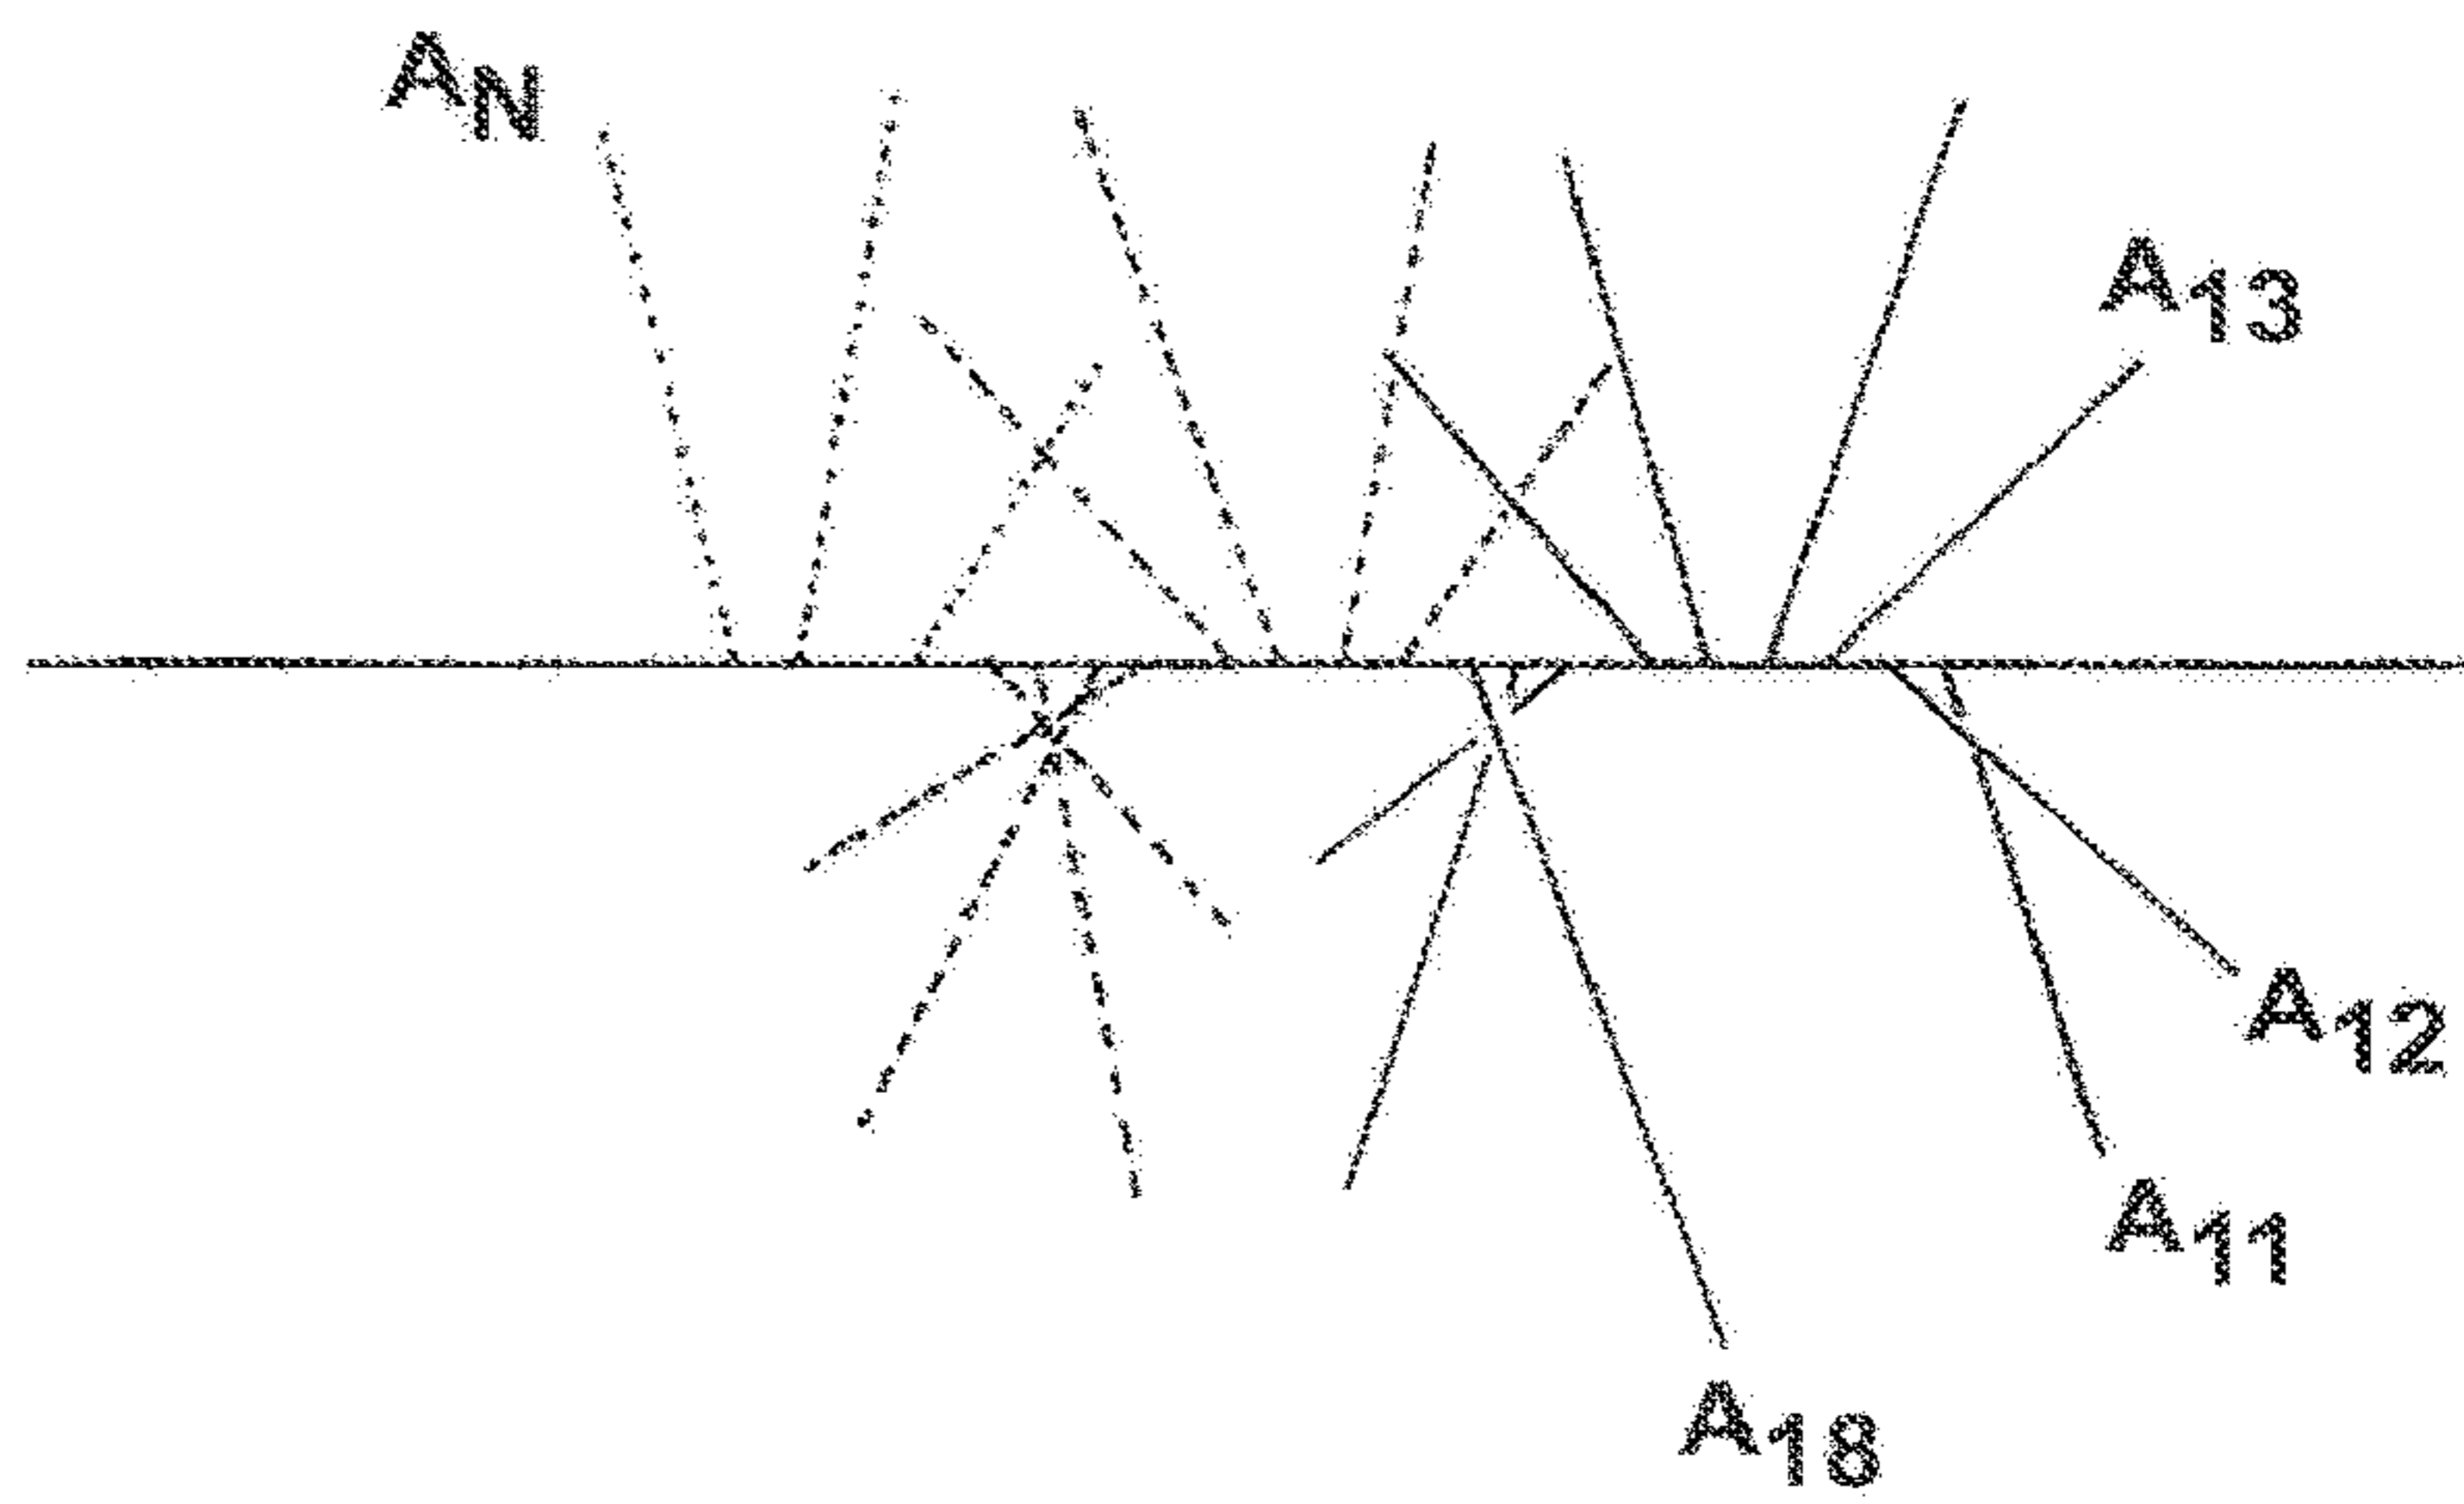


FIG. 9

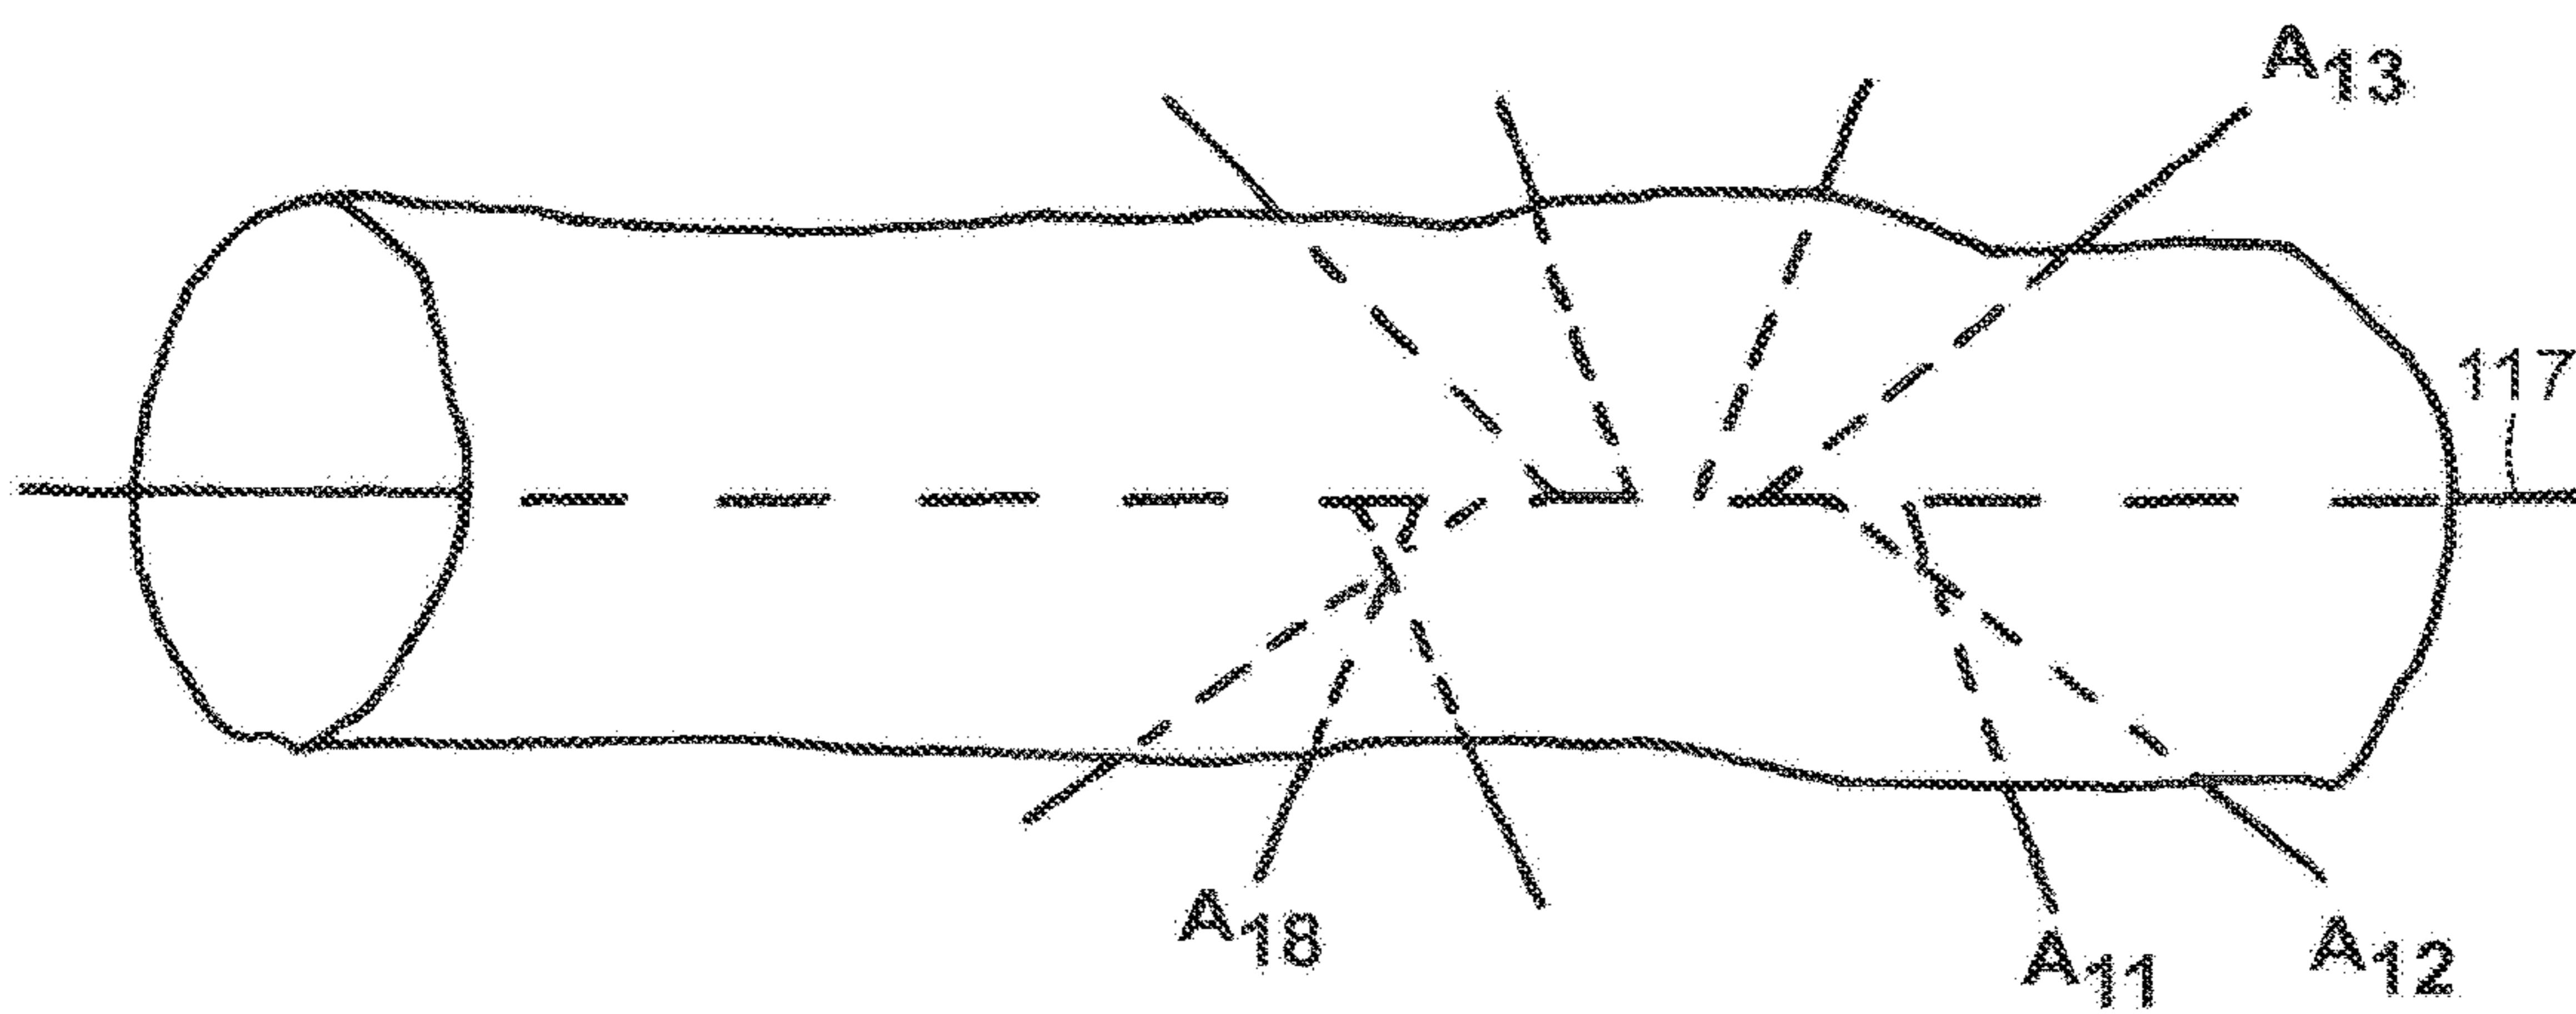
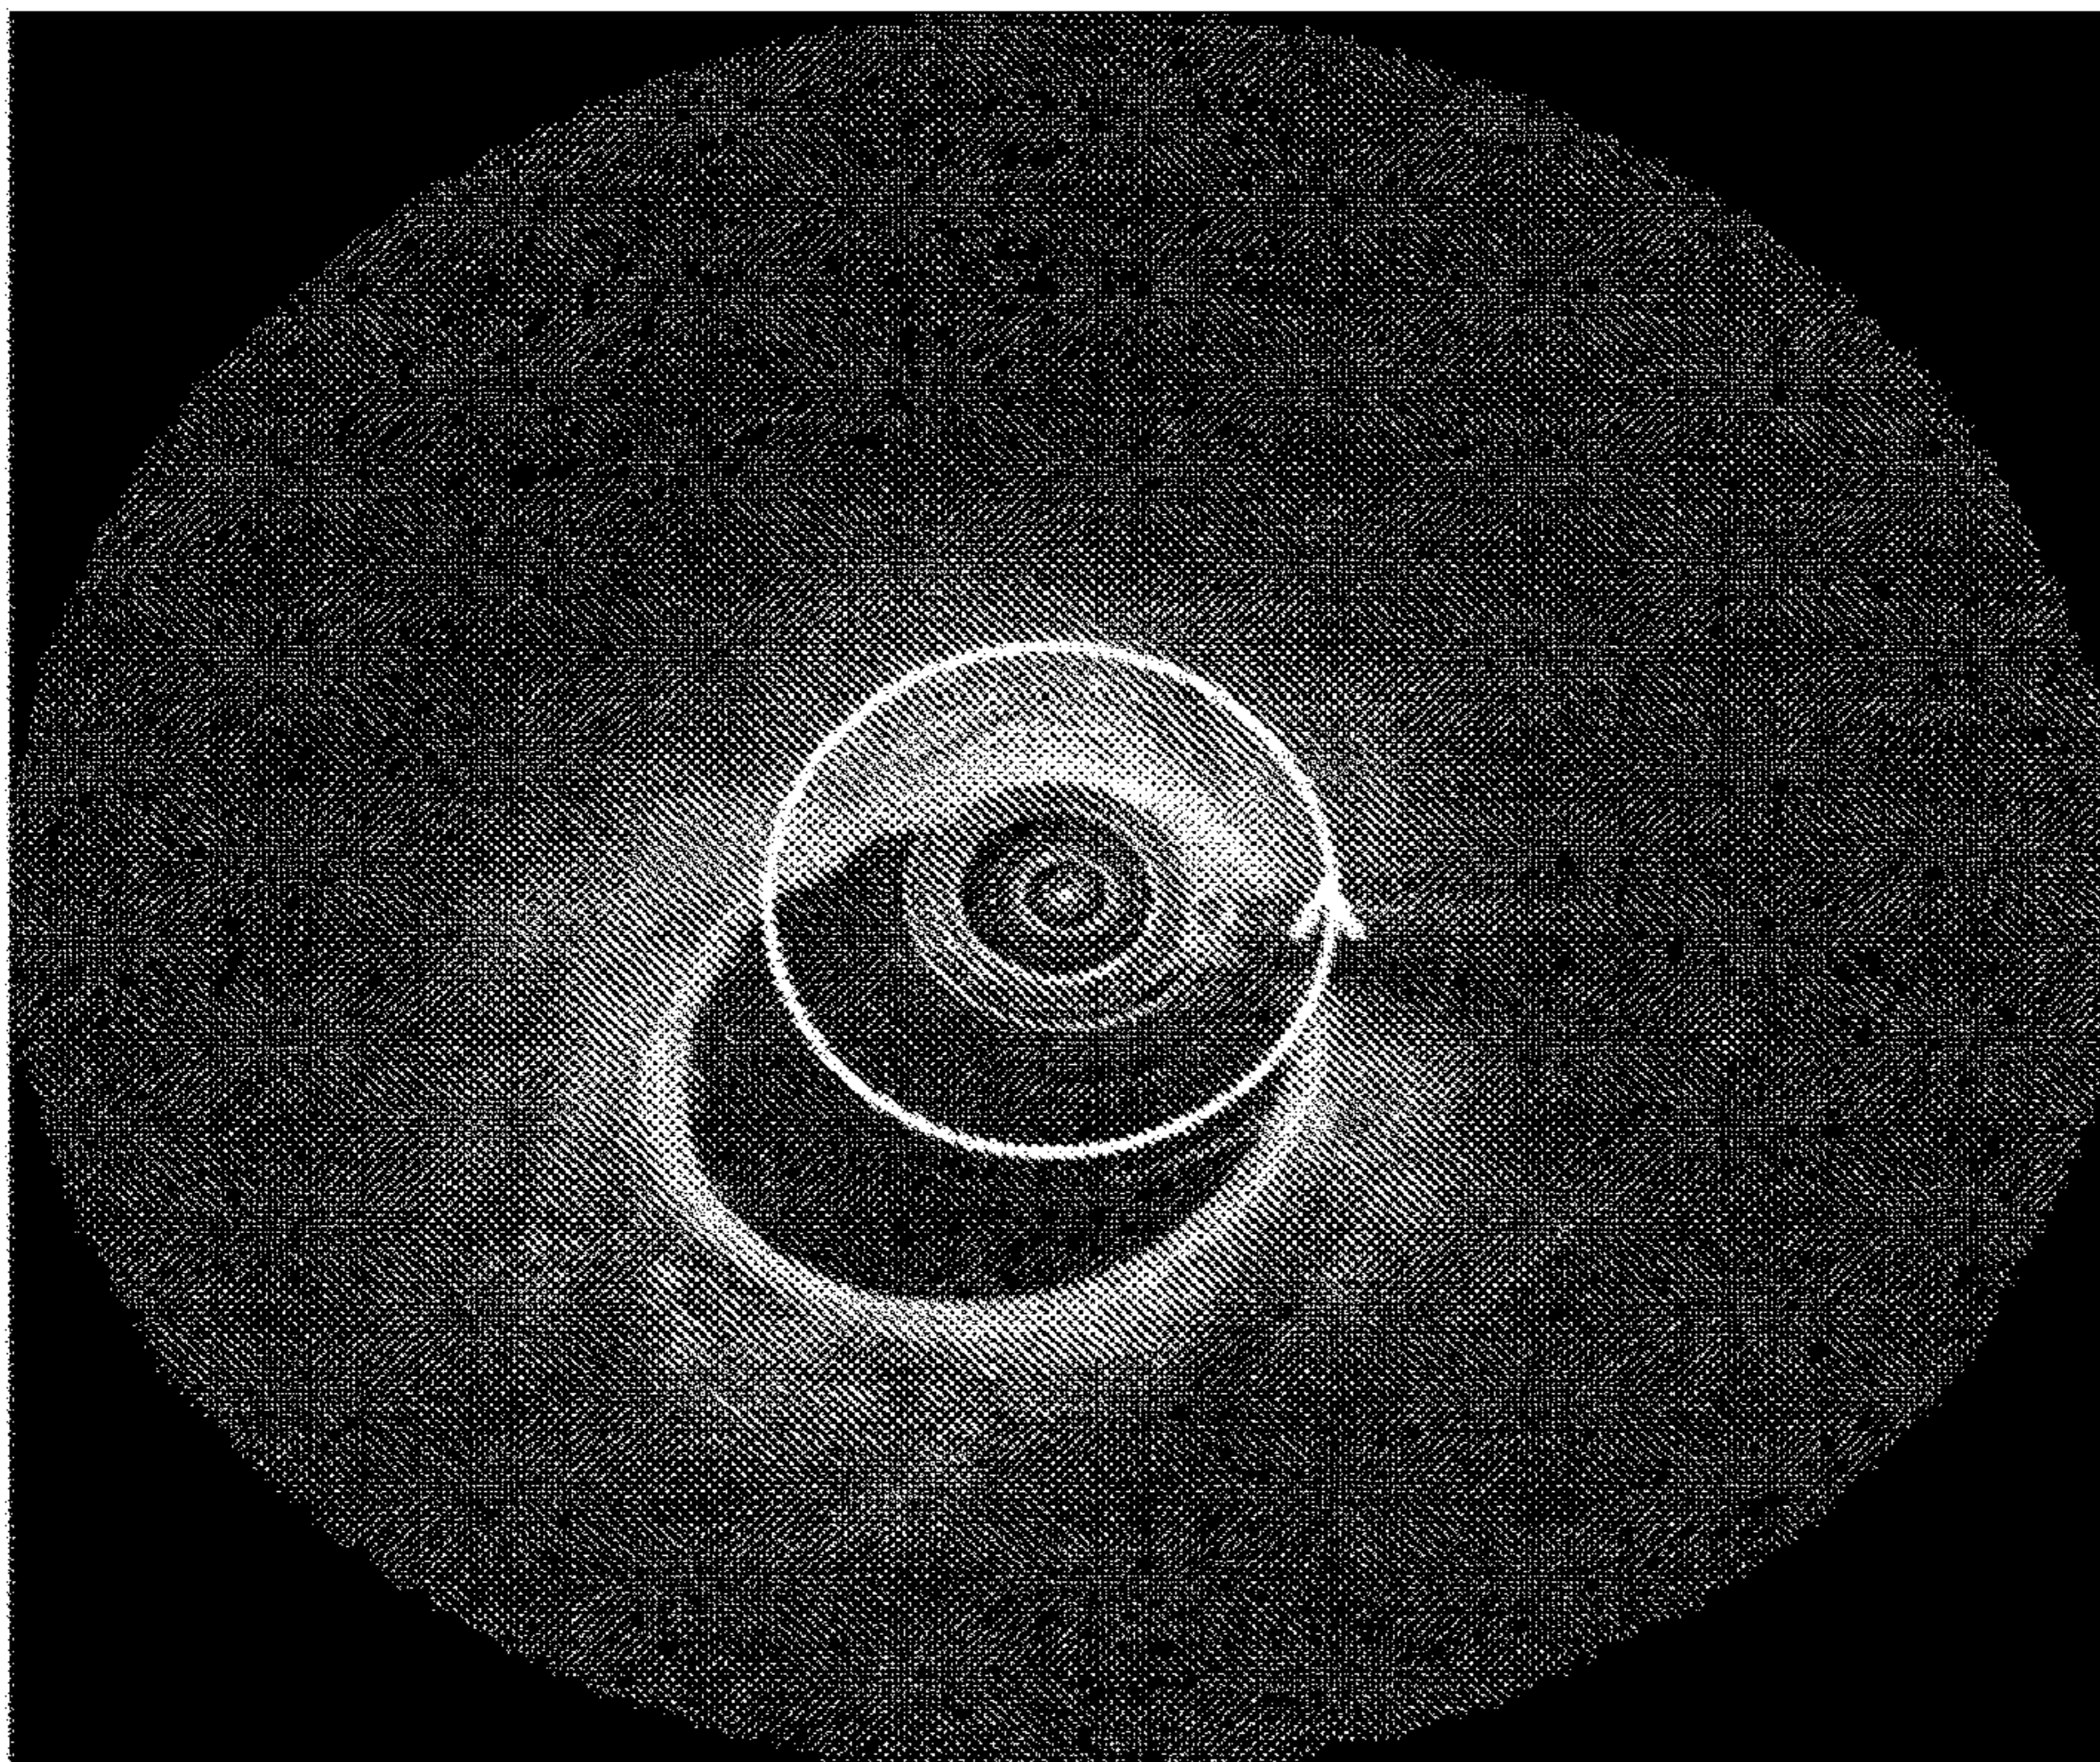
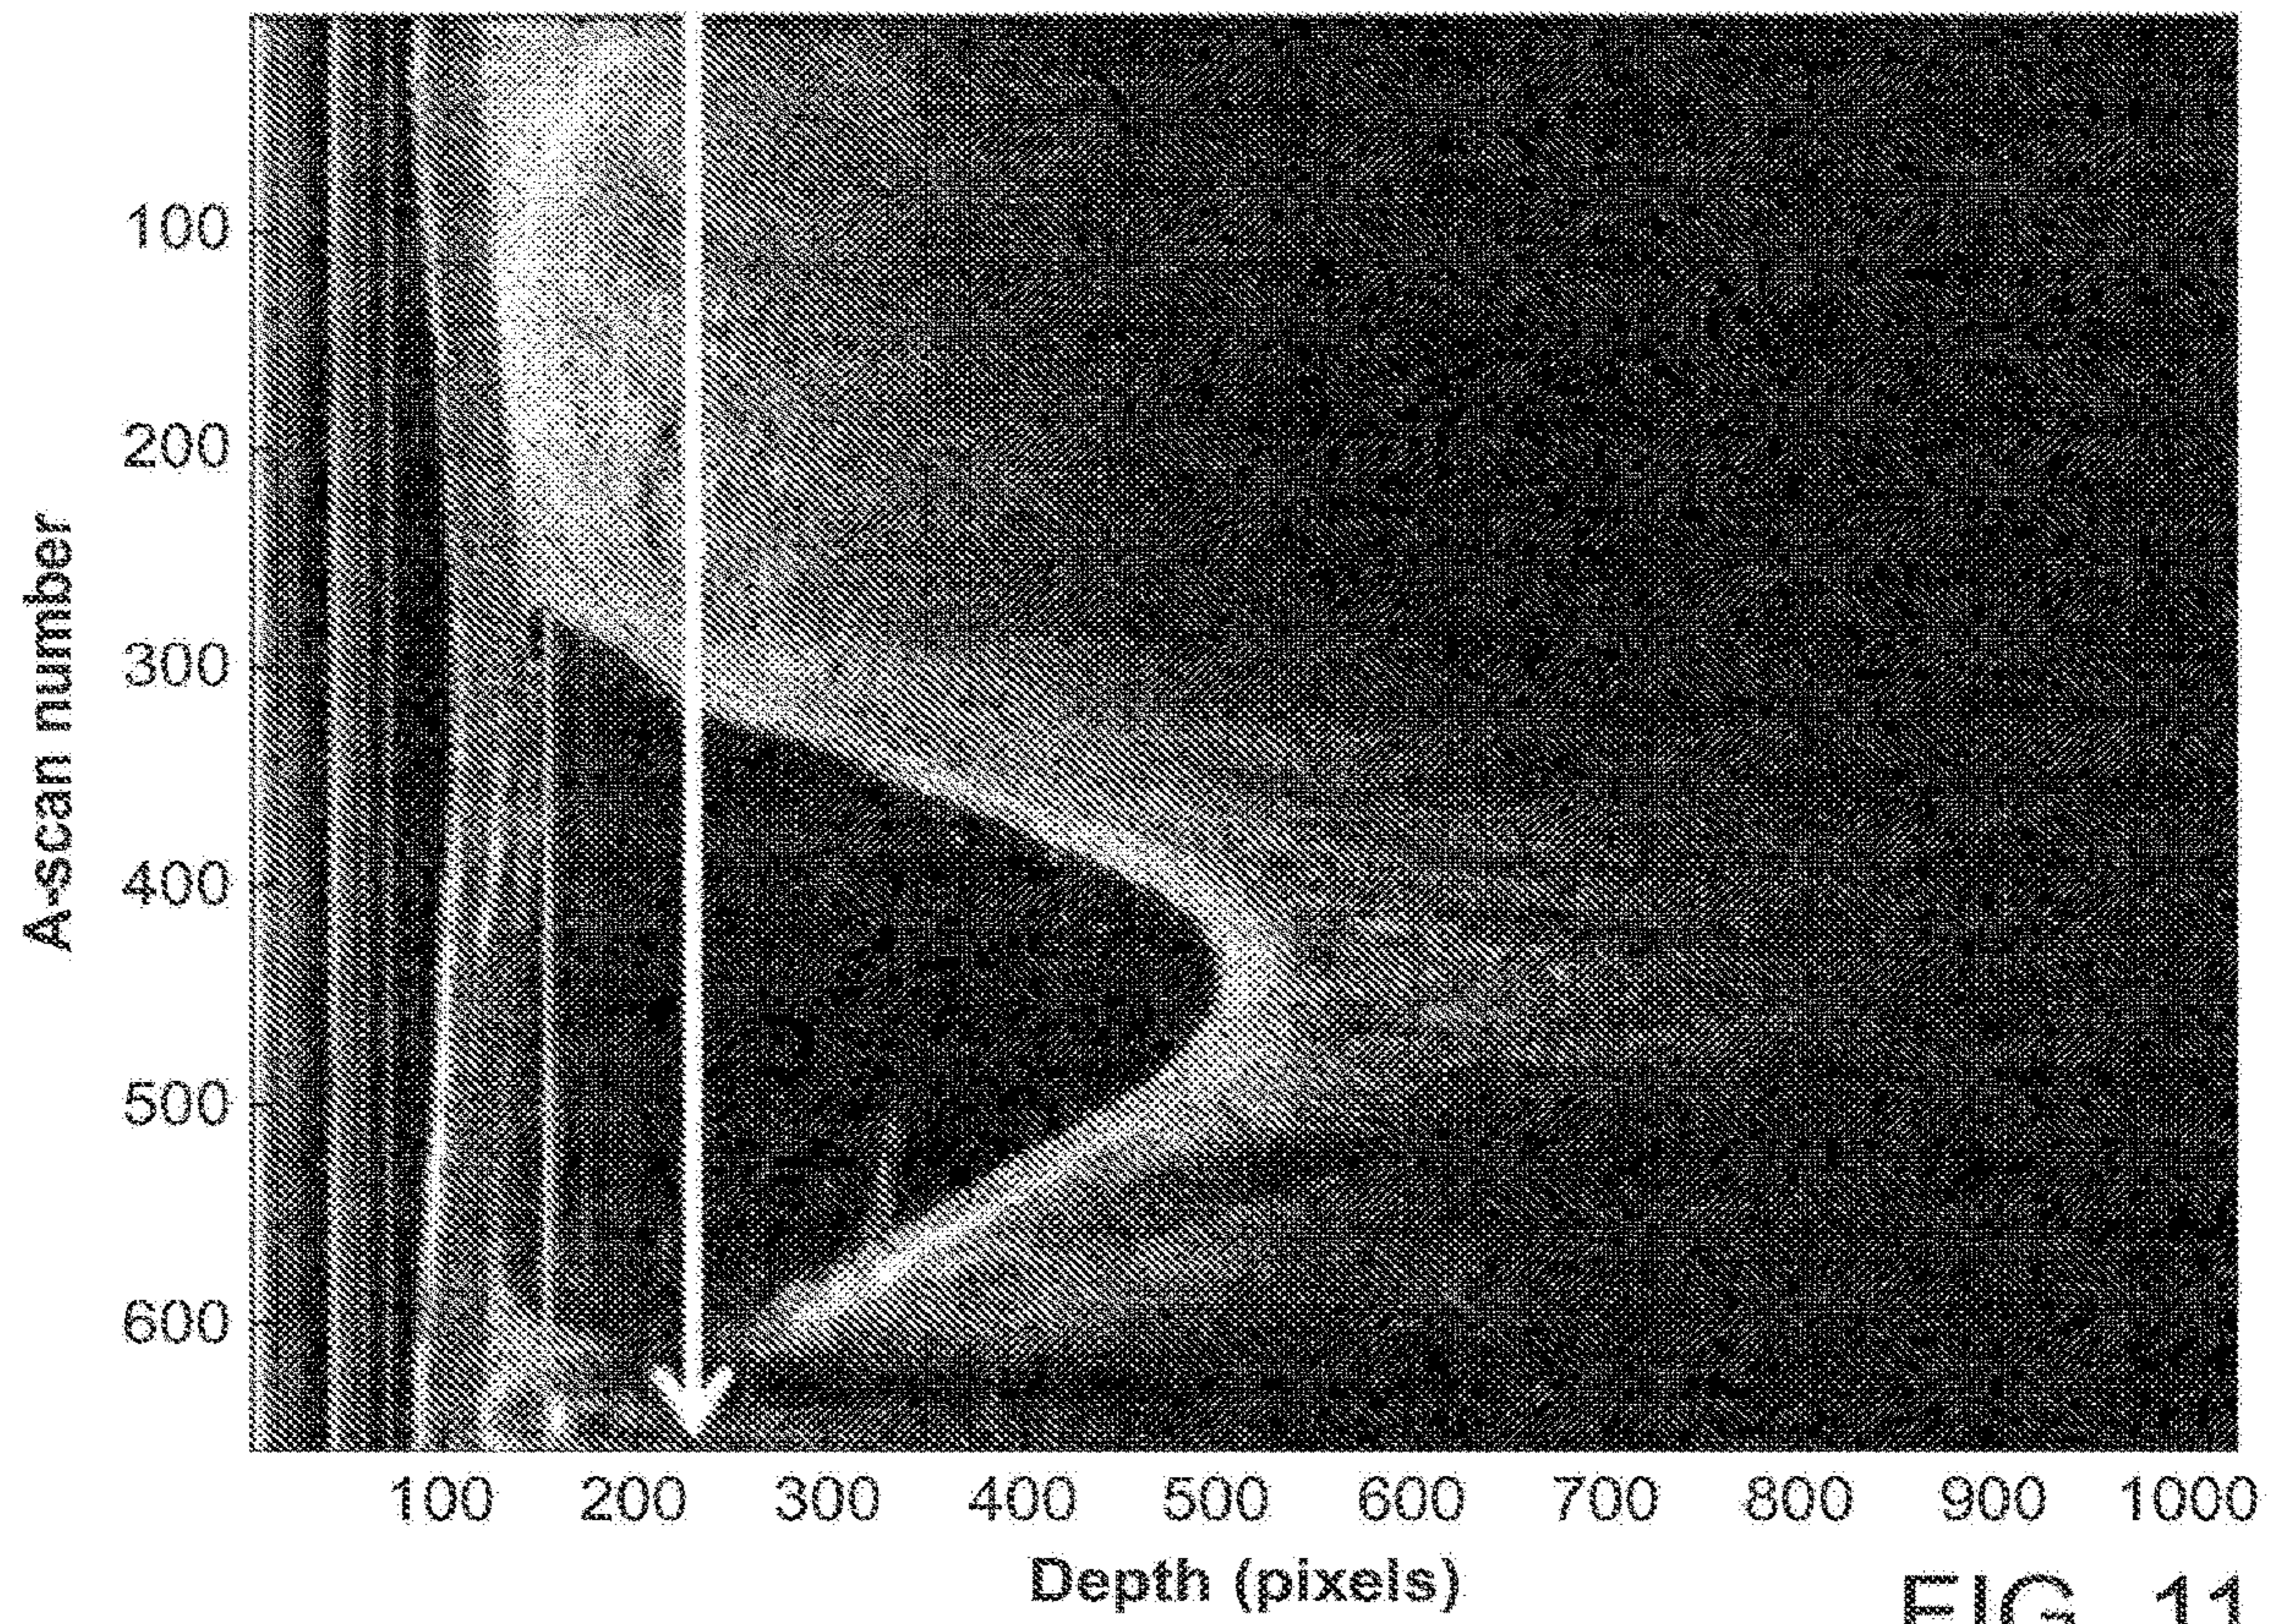


FIG. 10



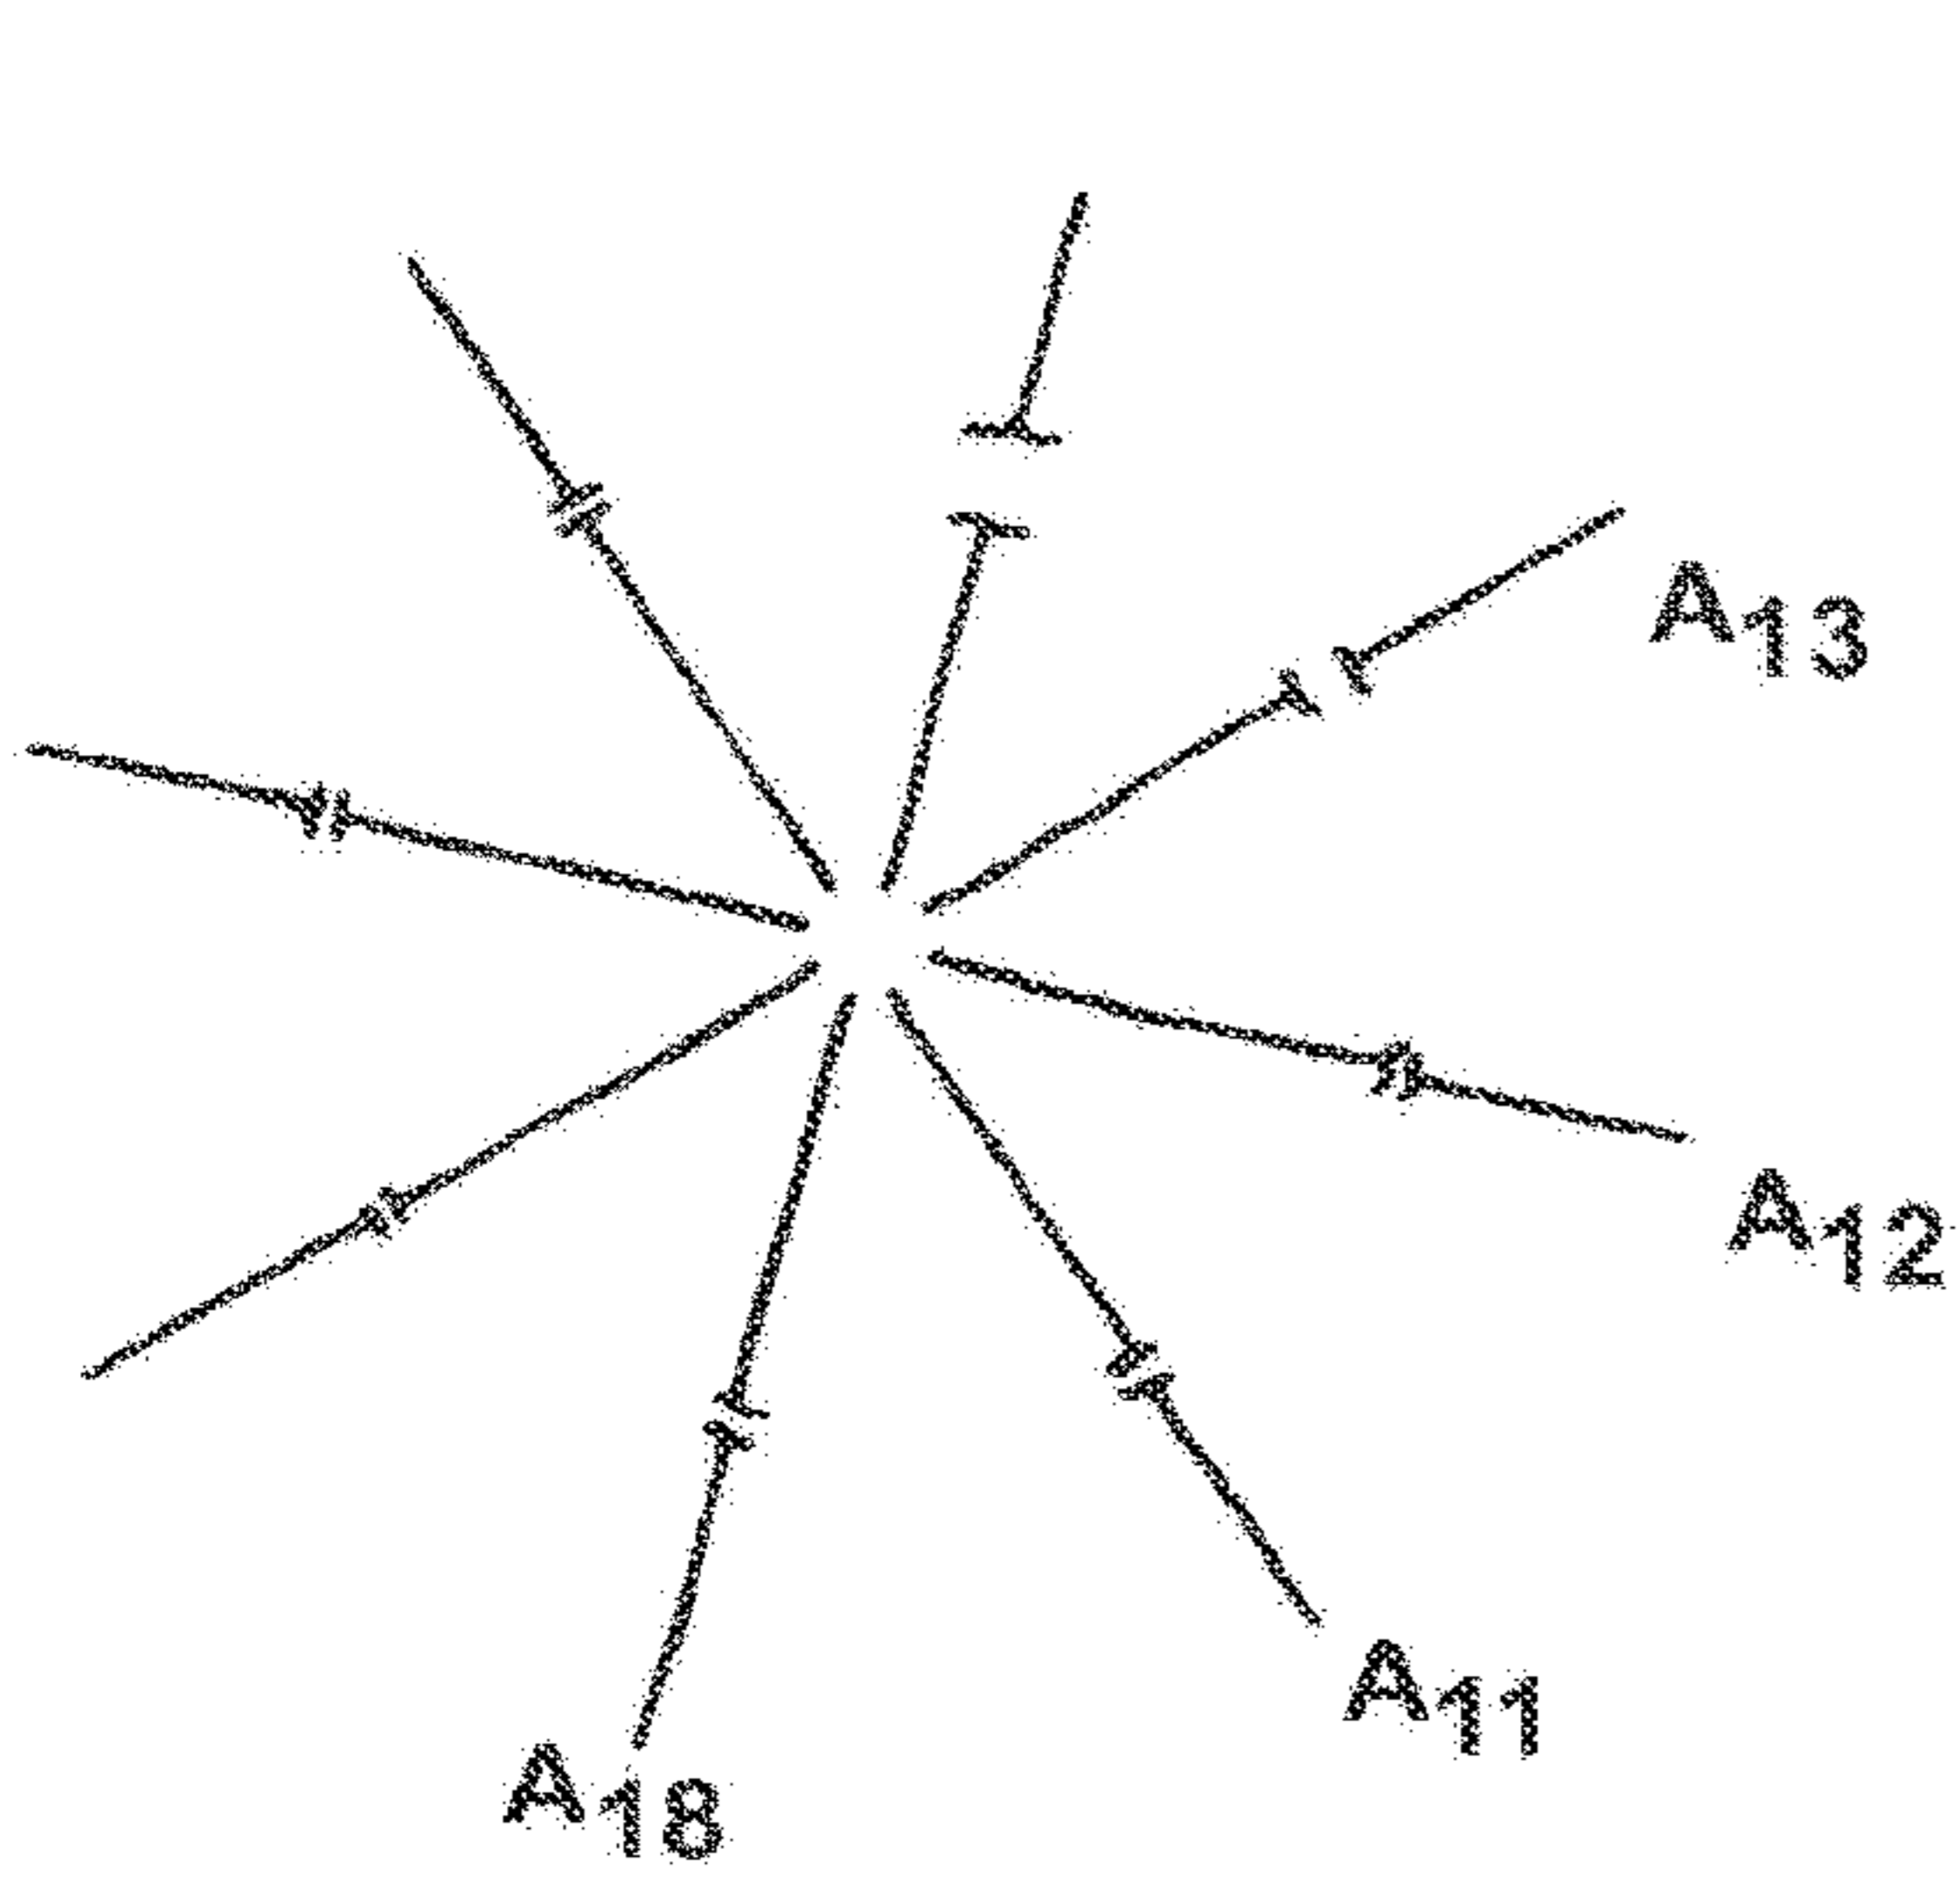


FIG. 13

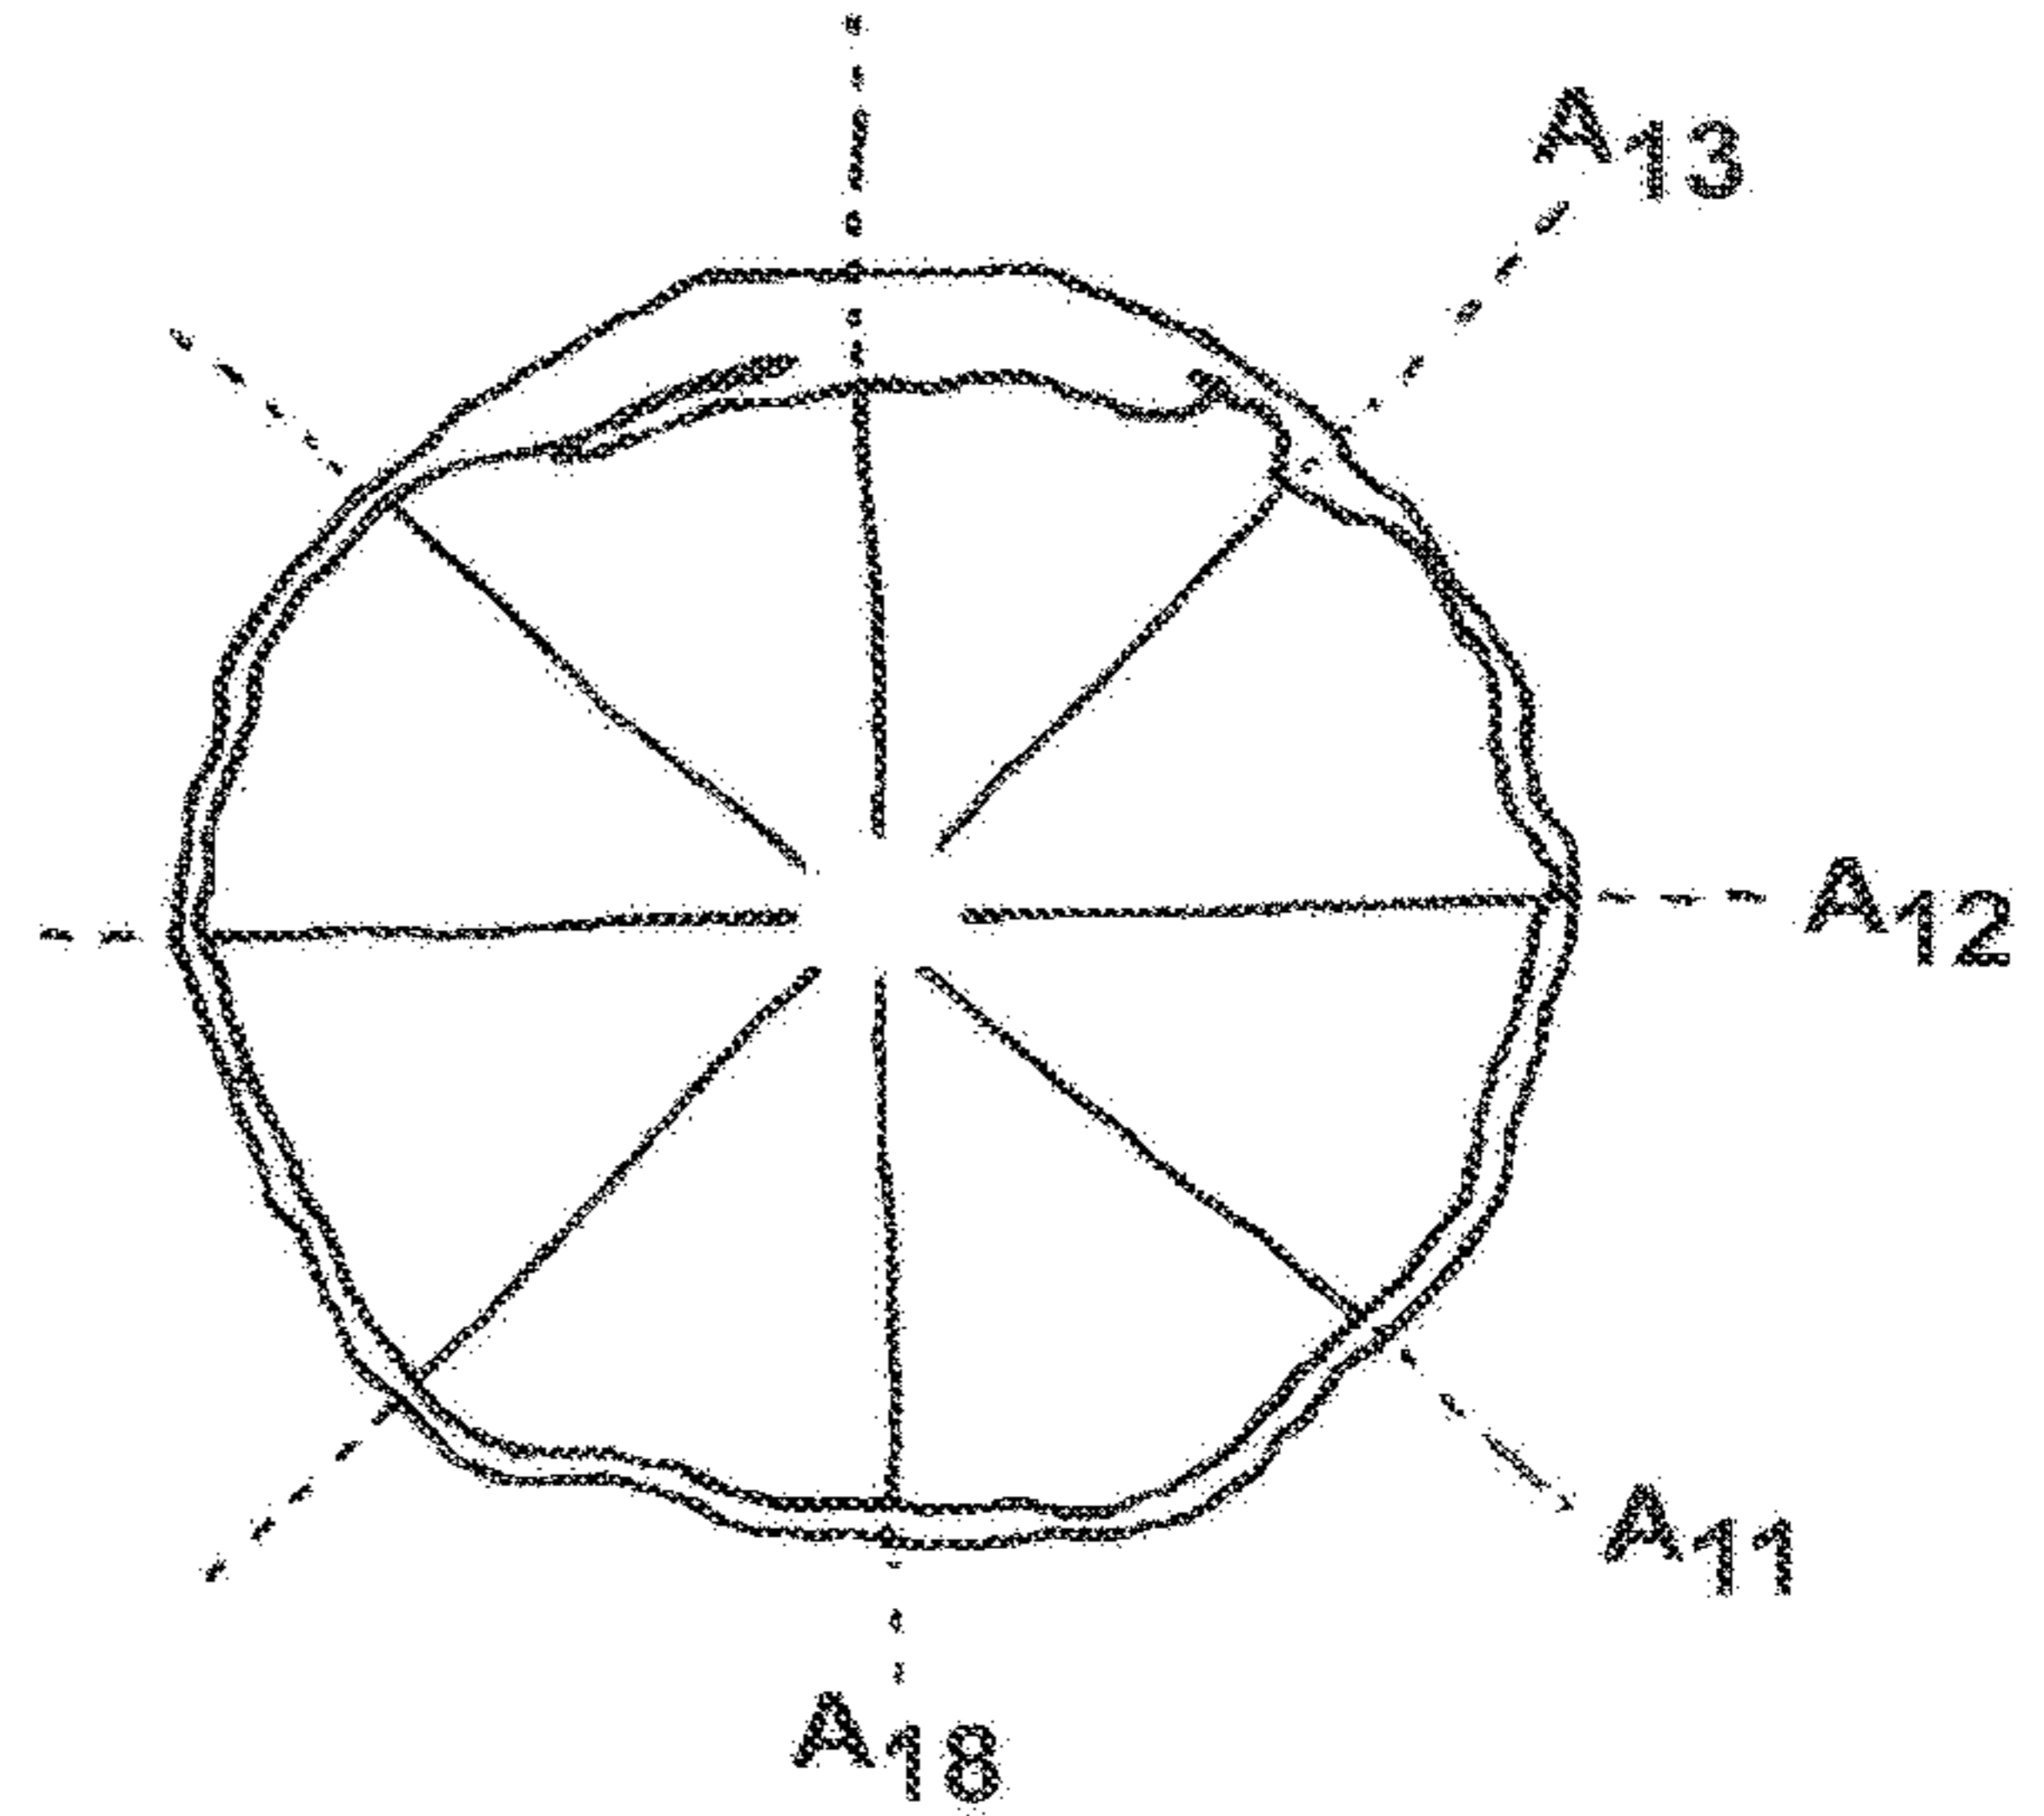


FIG. 14

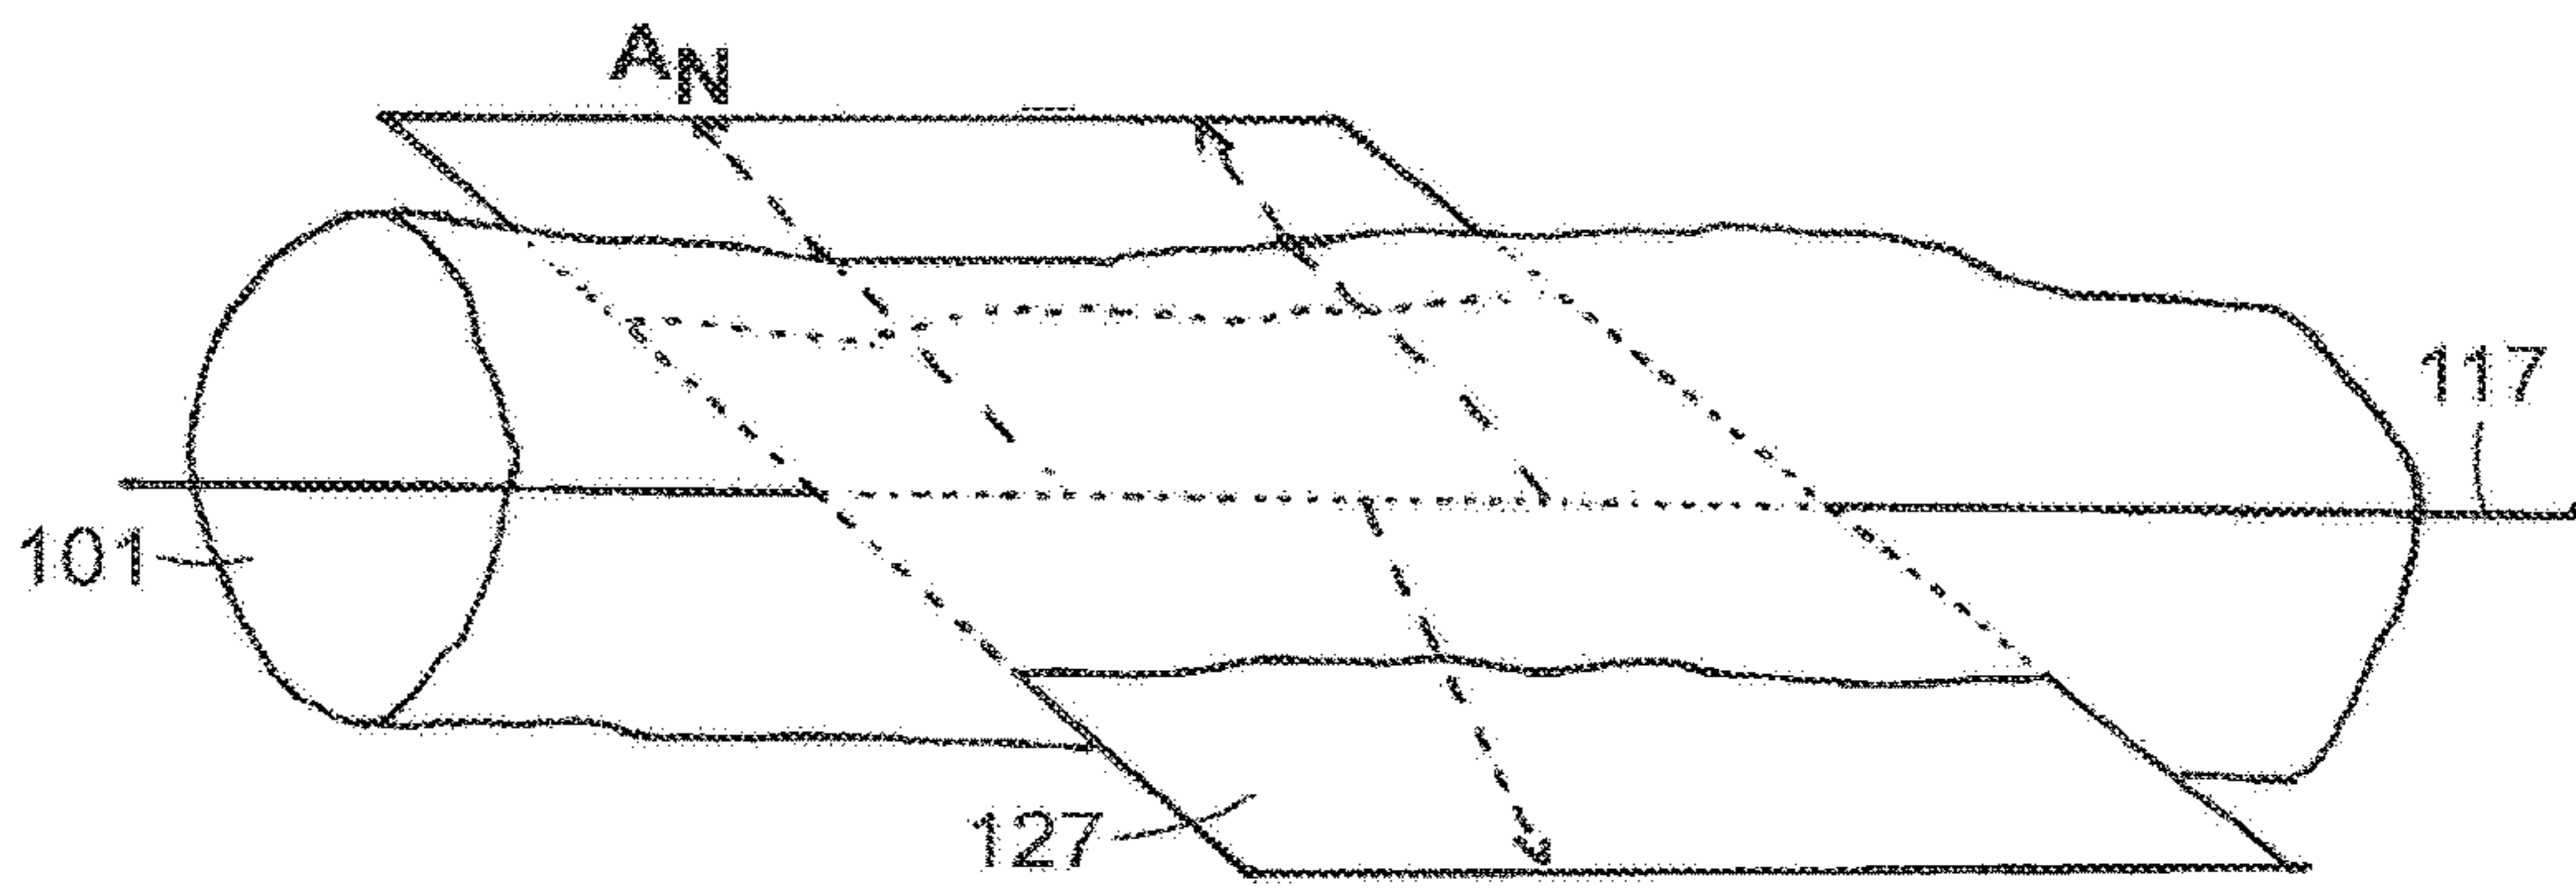


FIG. 15

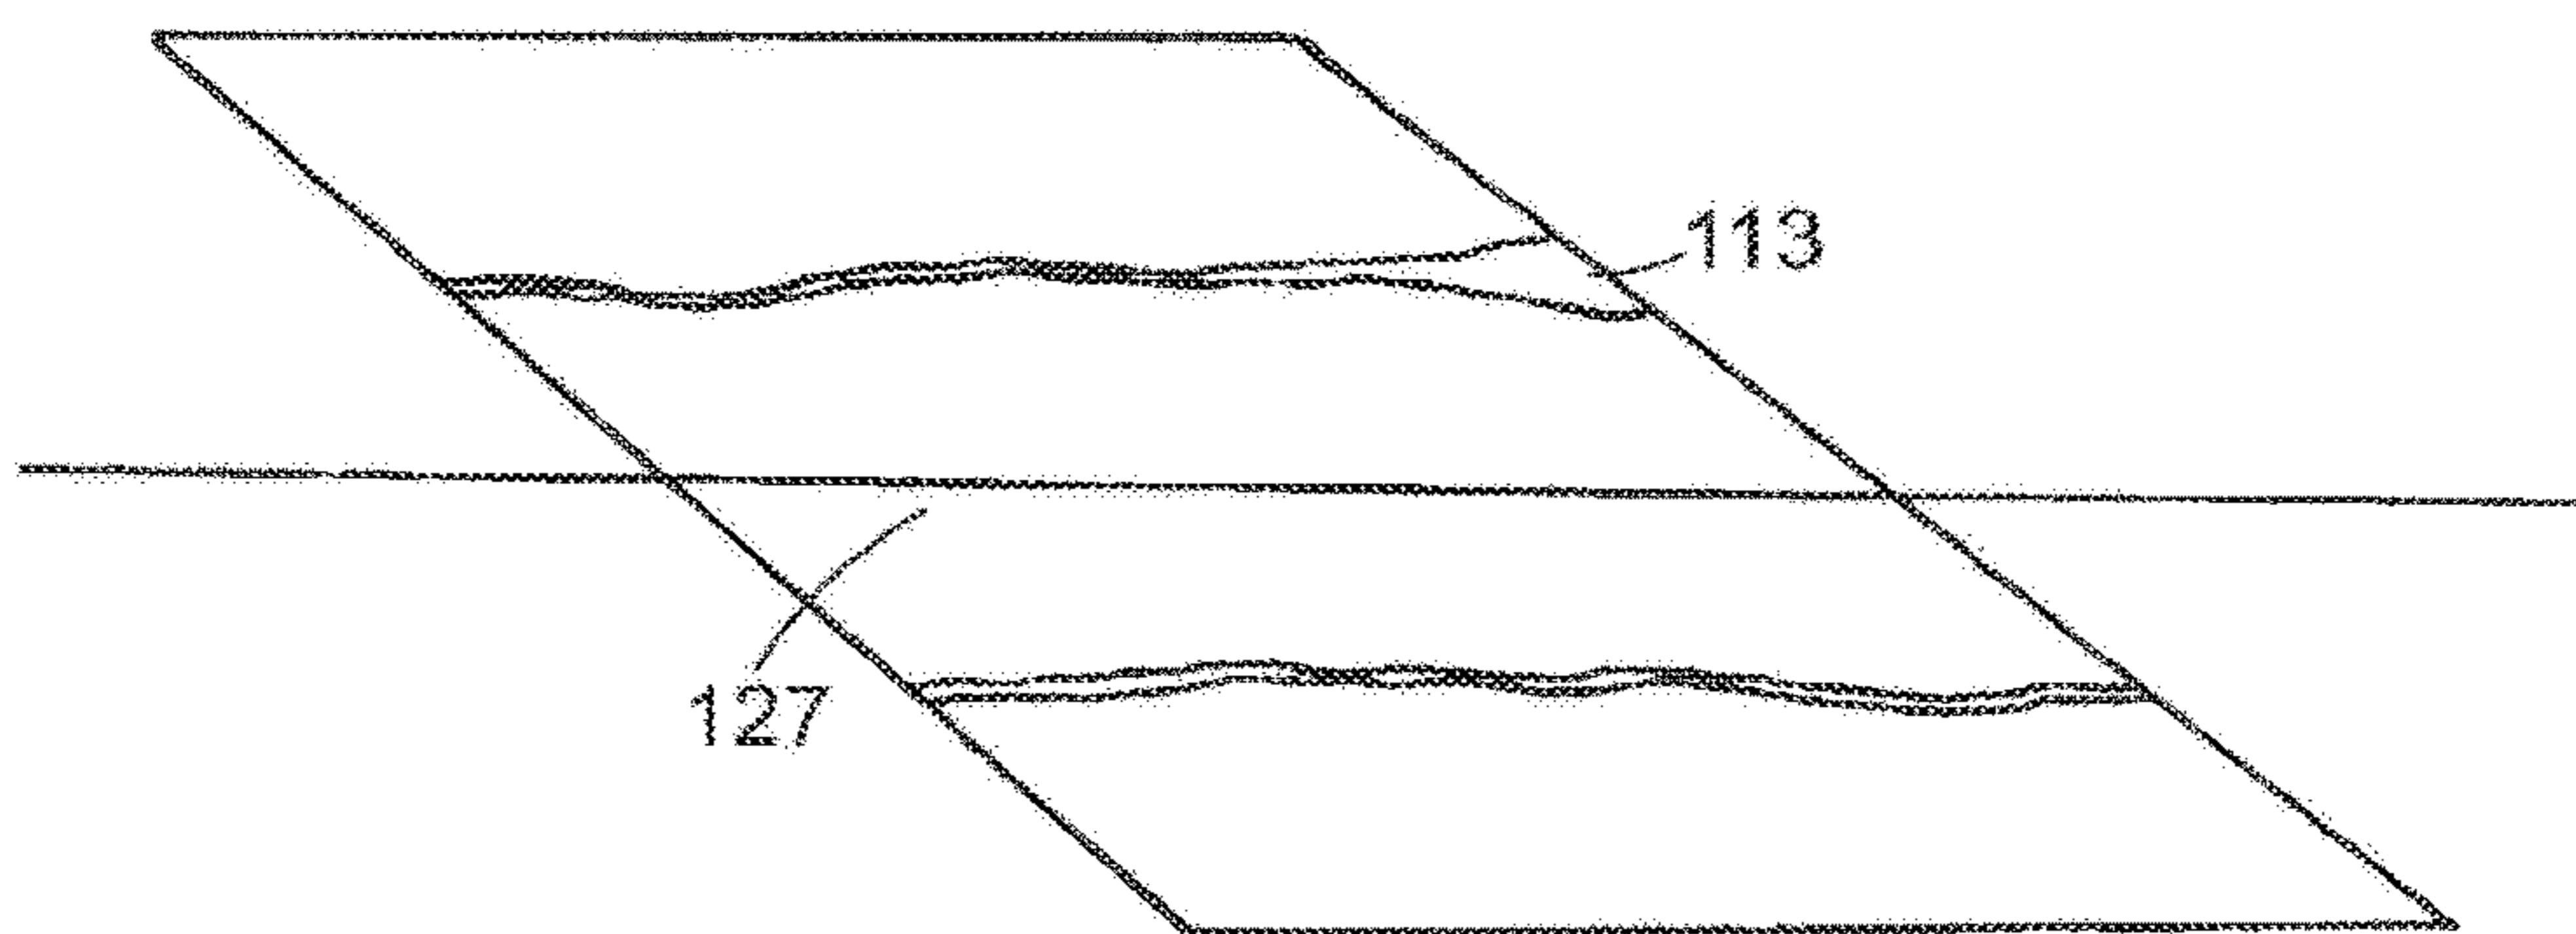


FIG. 16

VOLCANO

VL1: LAD Pre-Sie

v3.2 Test Case

12345678

OCT

10/15/2009 14:20:14

15-14

Case Explorer

Frames: 10

Loops: 2

Area1-Frame: 1514

Area: 19.5 mm²

Min Dia: 4.9 mm

Max Dia: 5.1 mm

Difference

14.5mm=(74.2%)

Area2-Frame: 1514

Area: 5.0 mm²

Min Dia: 2.3 mm

Max Dia: 2.9 mm

Live

Diameter

Draw

1mm

PullBack: 80.1 mm

1514

TARGET ASSIST

Selected Mode

Patient

Home

VH

End Case

Archive

Retrieve

Live

Diameter

Draw

Dots

Delete

Press Measure for Autoborders or Select from Measurement Toolbar

FIG. 17

237

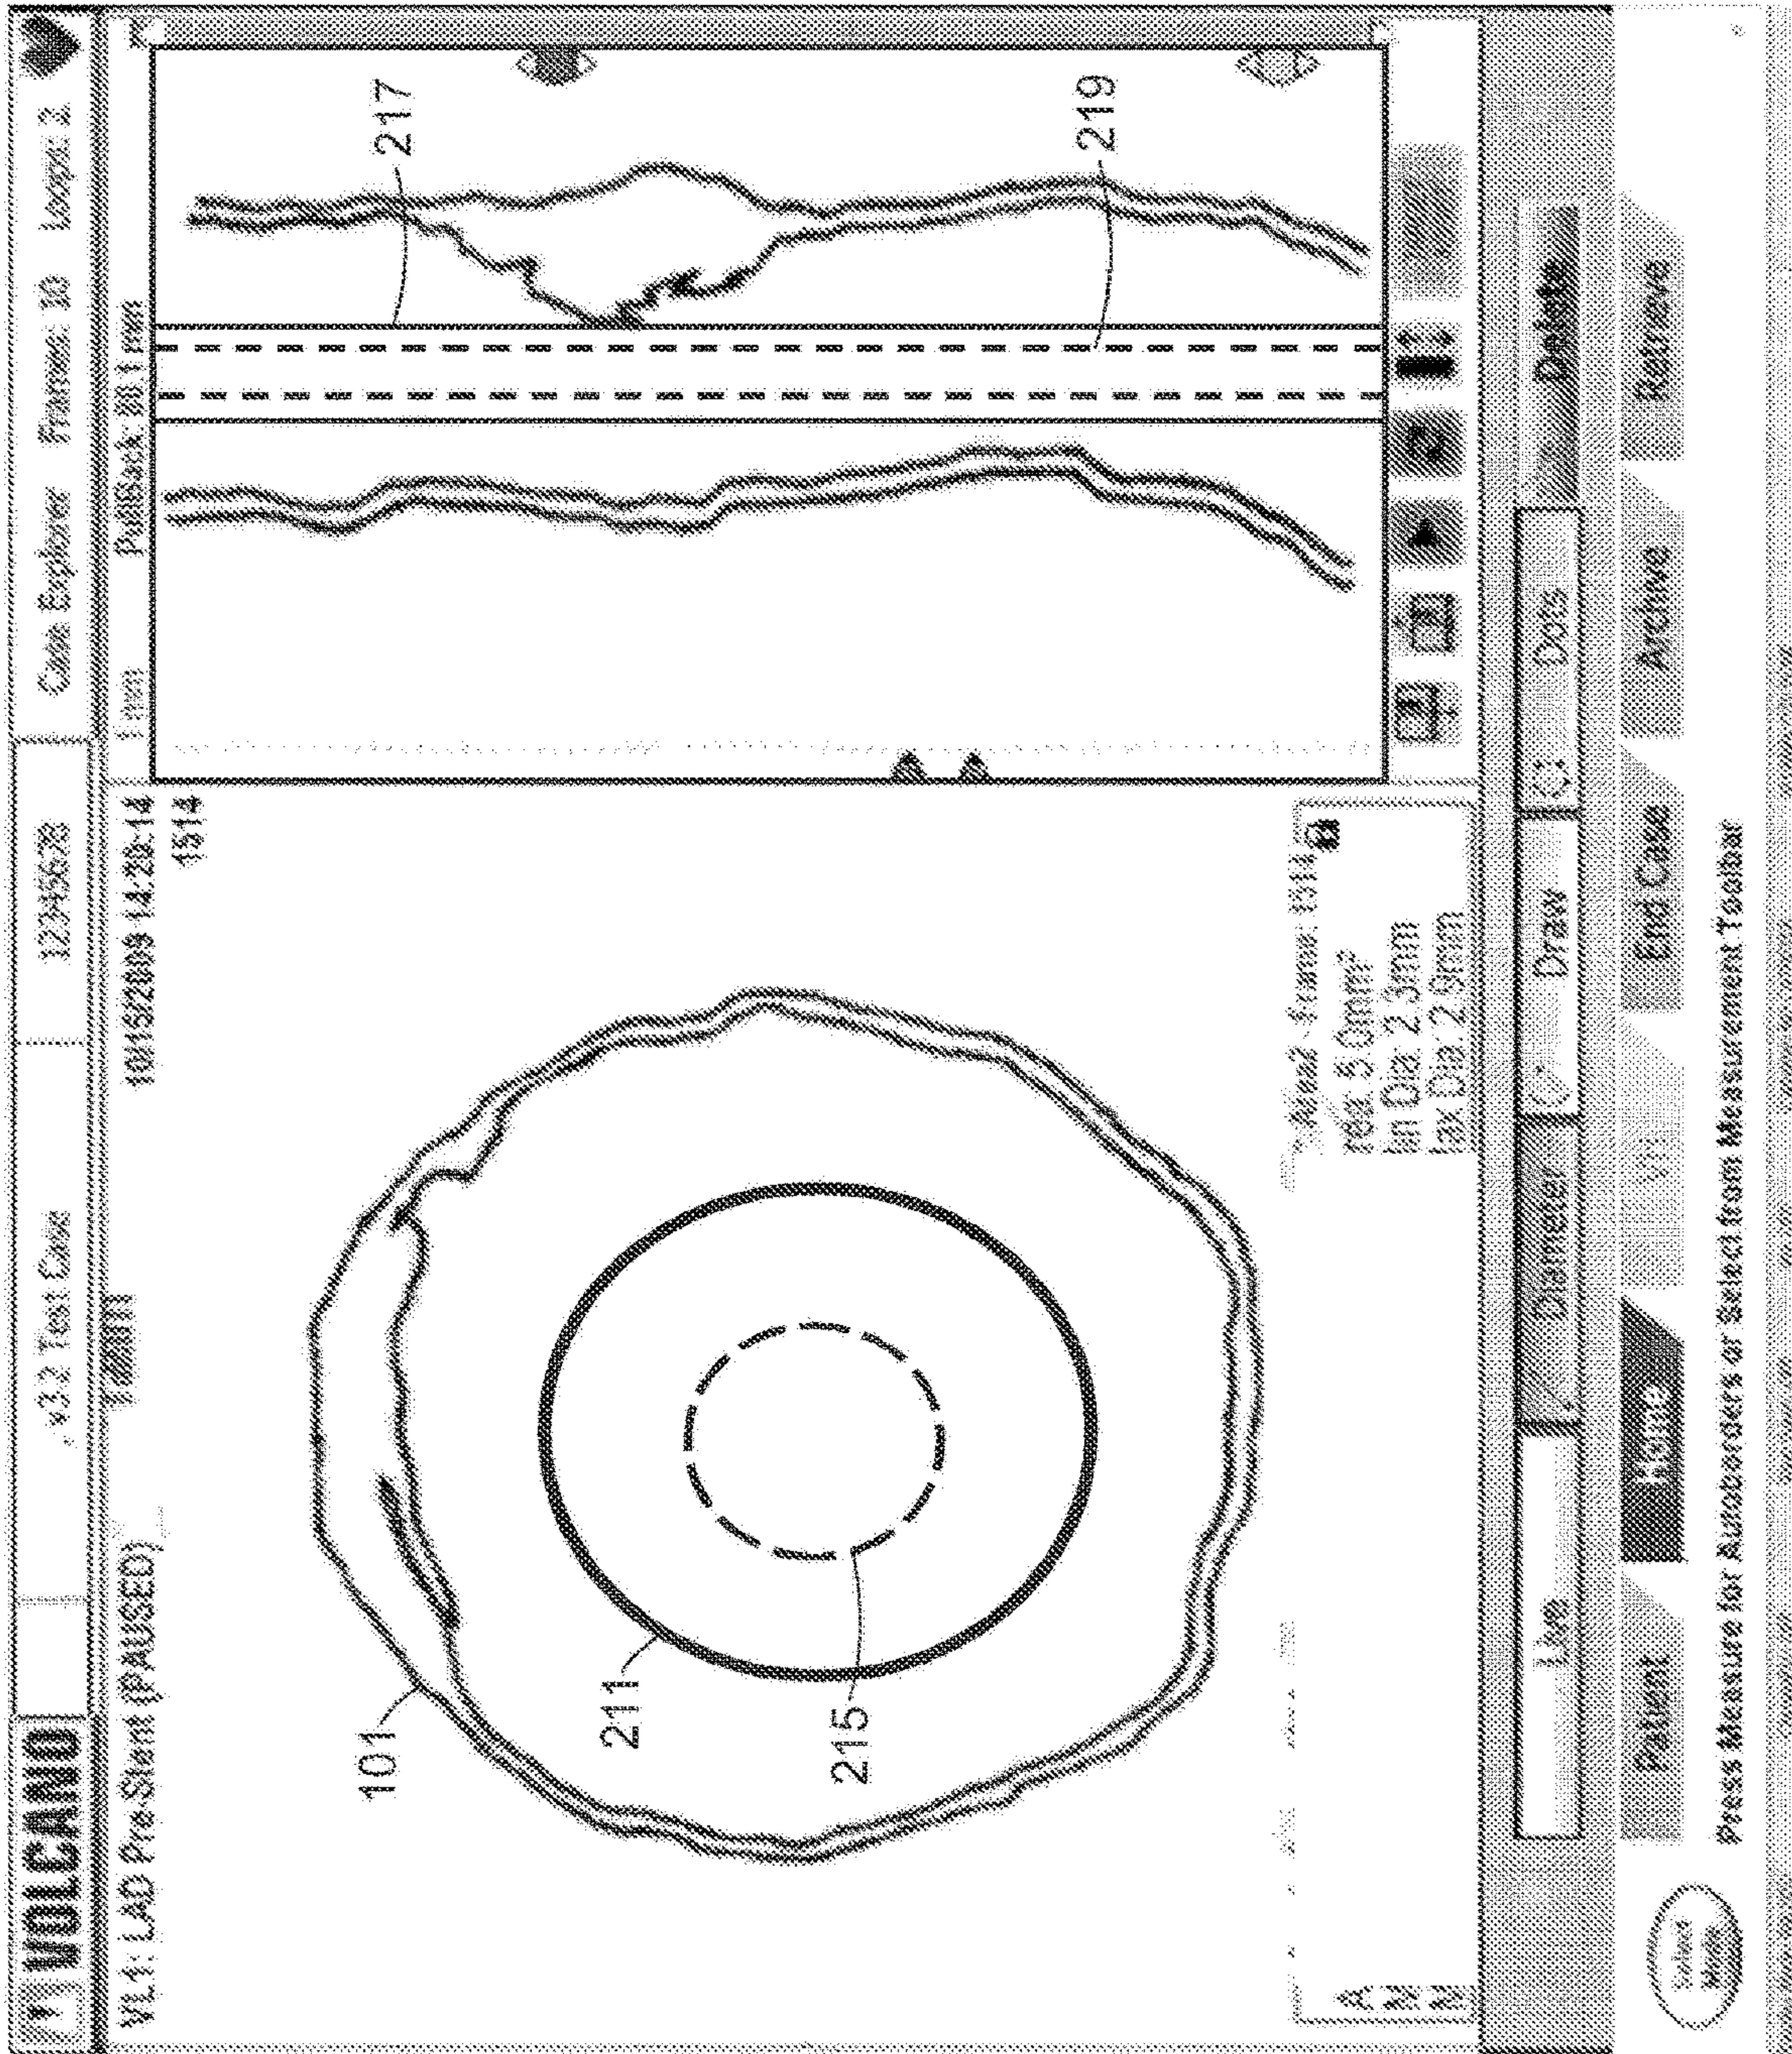


FIG. 18

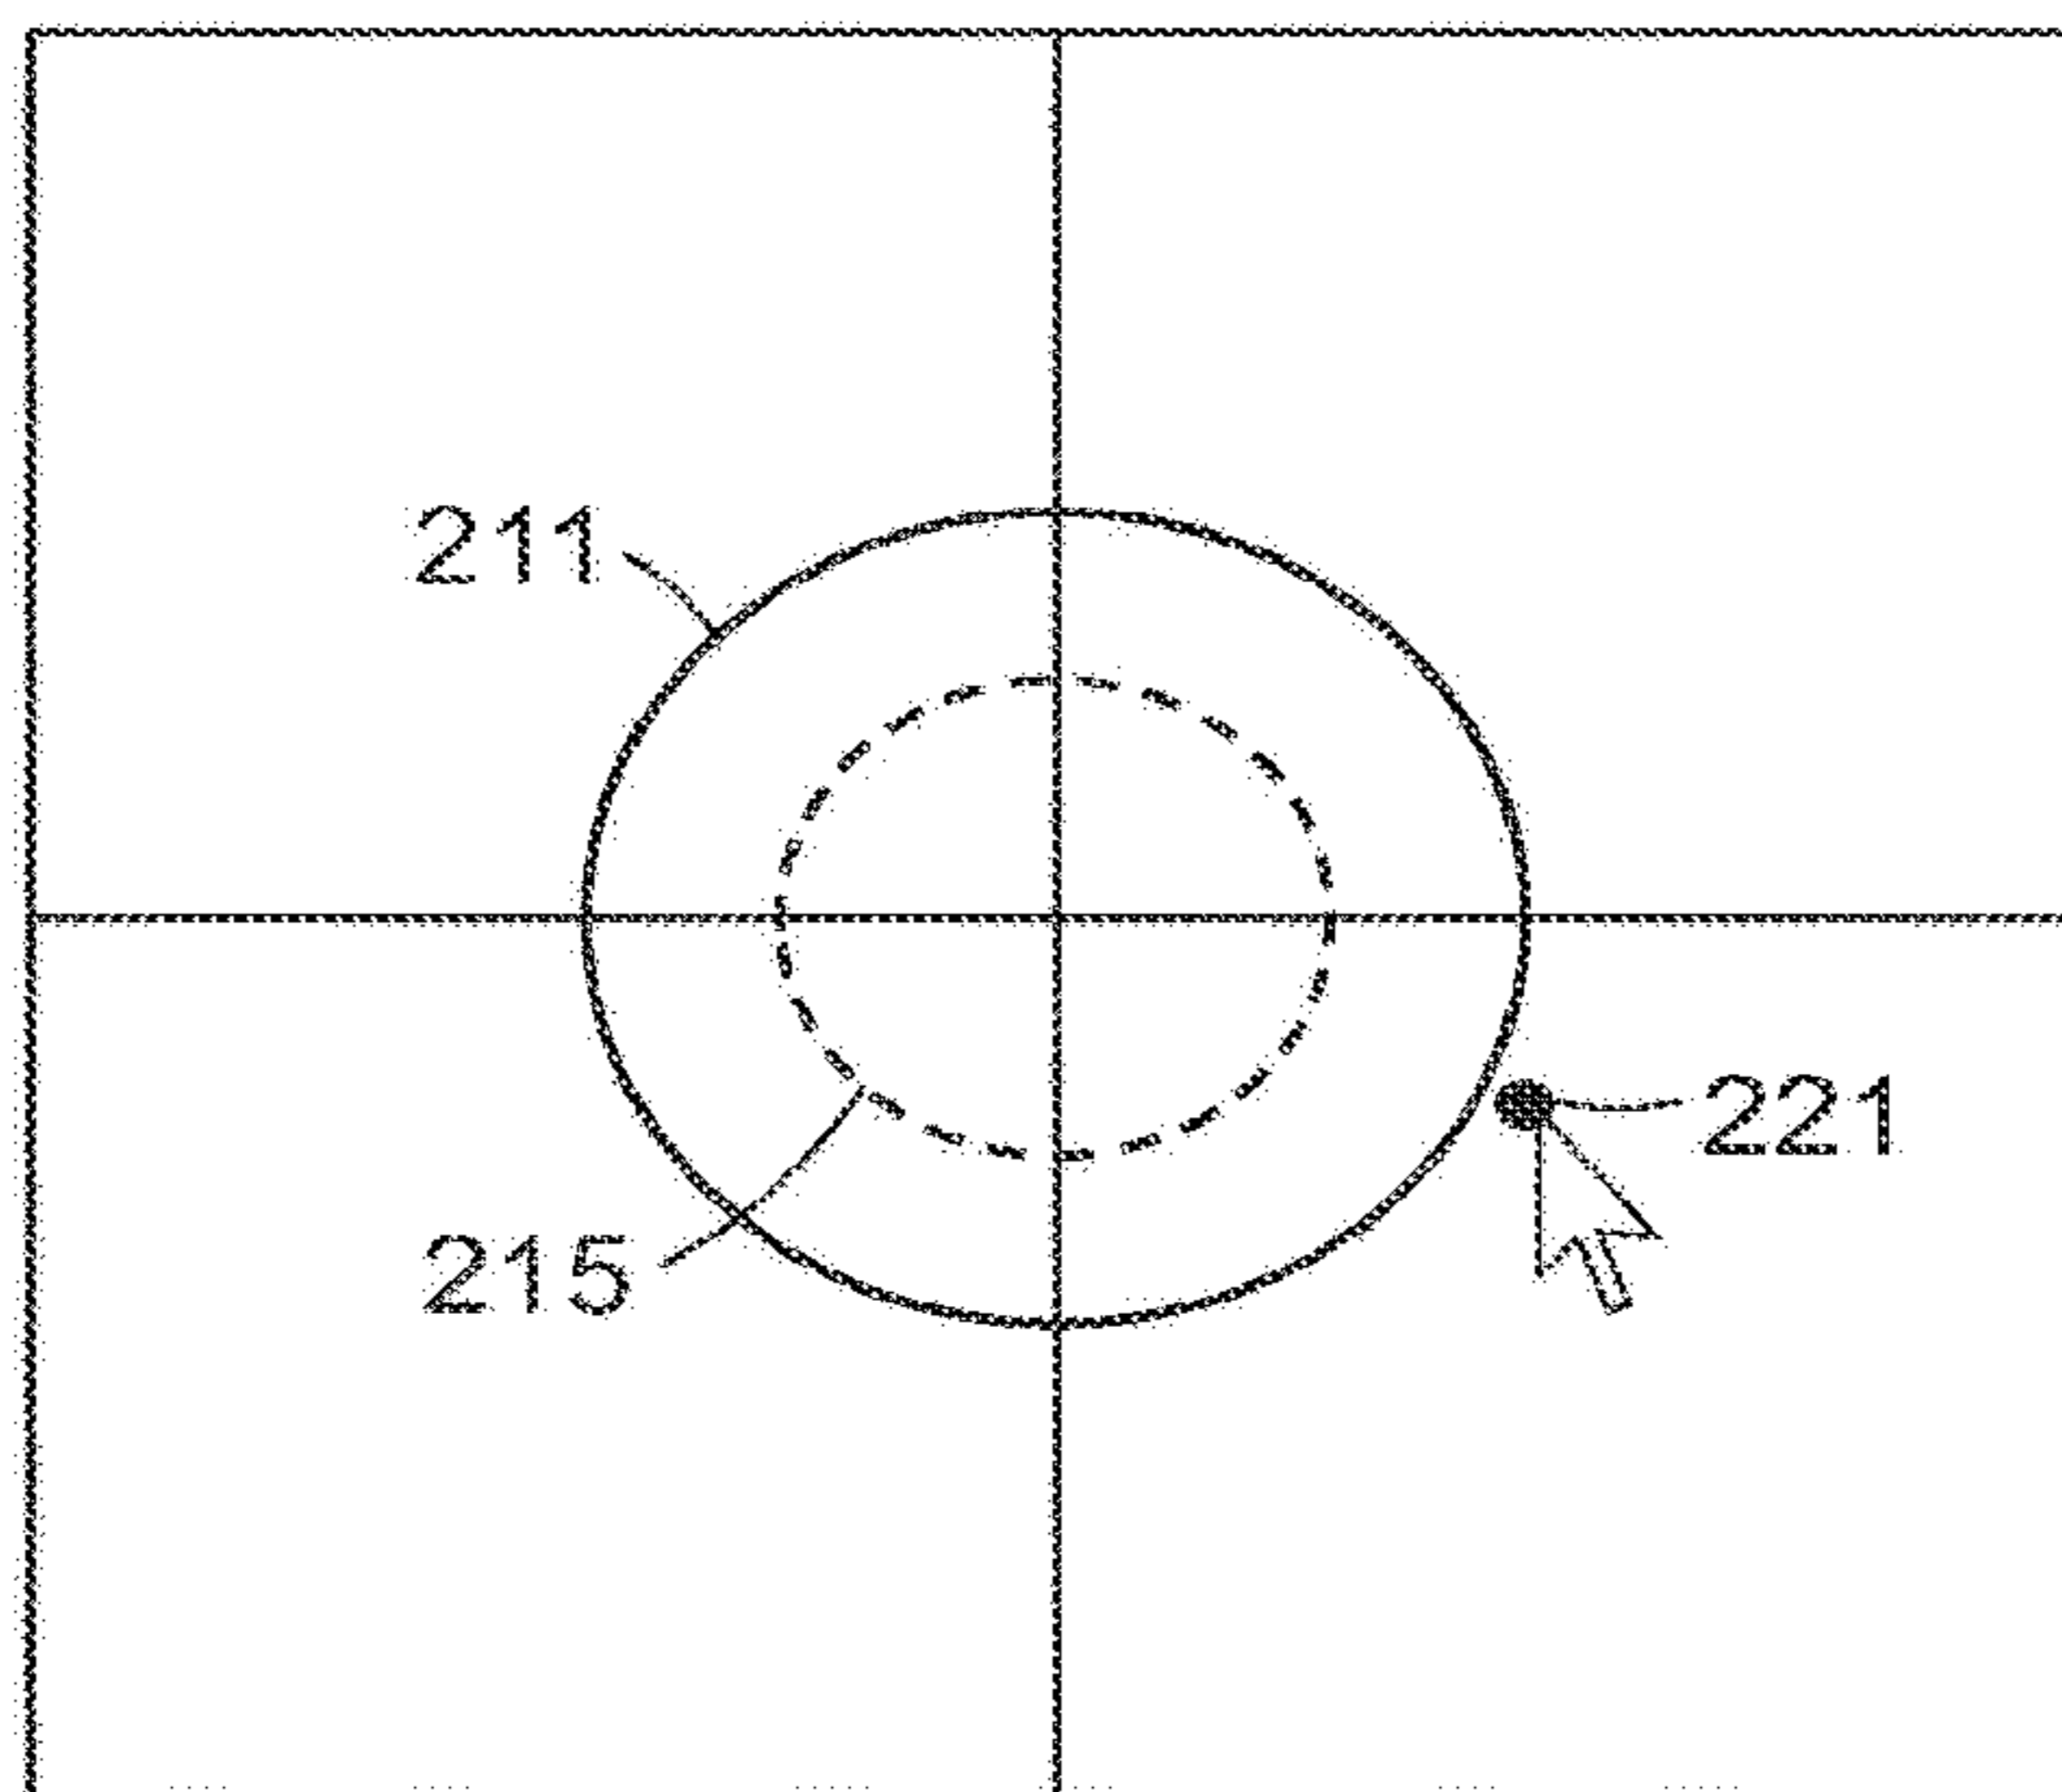


FIG. 19

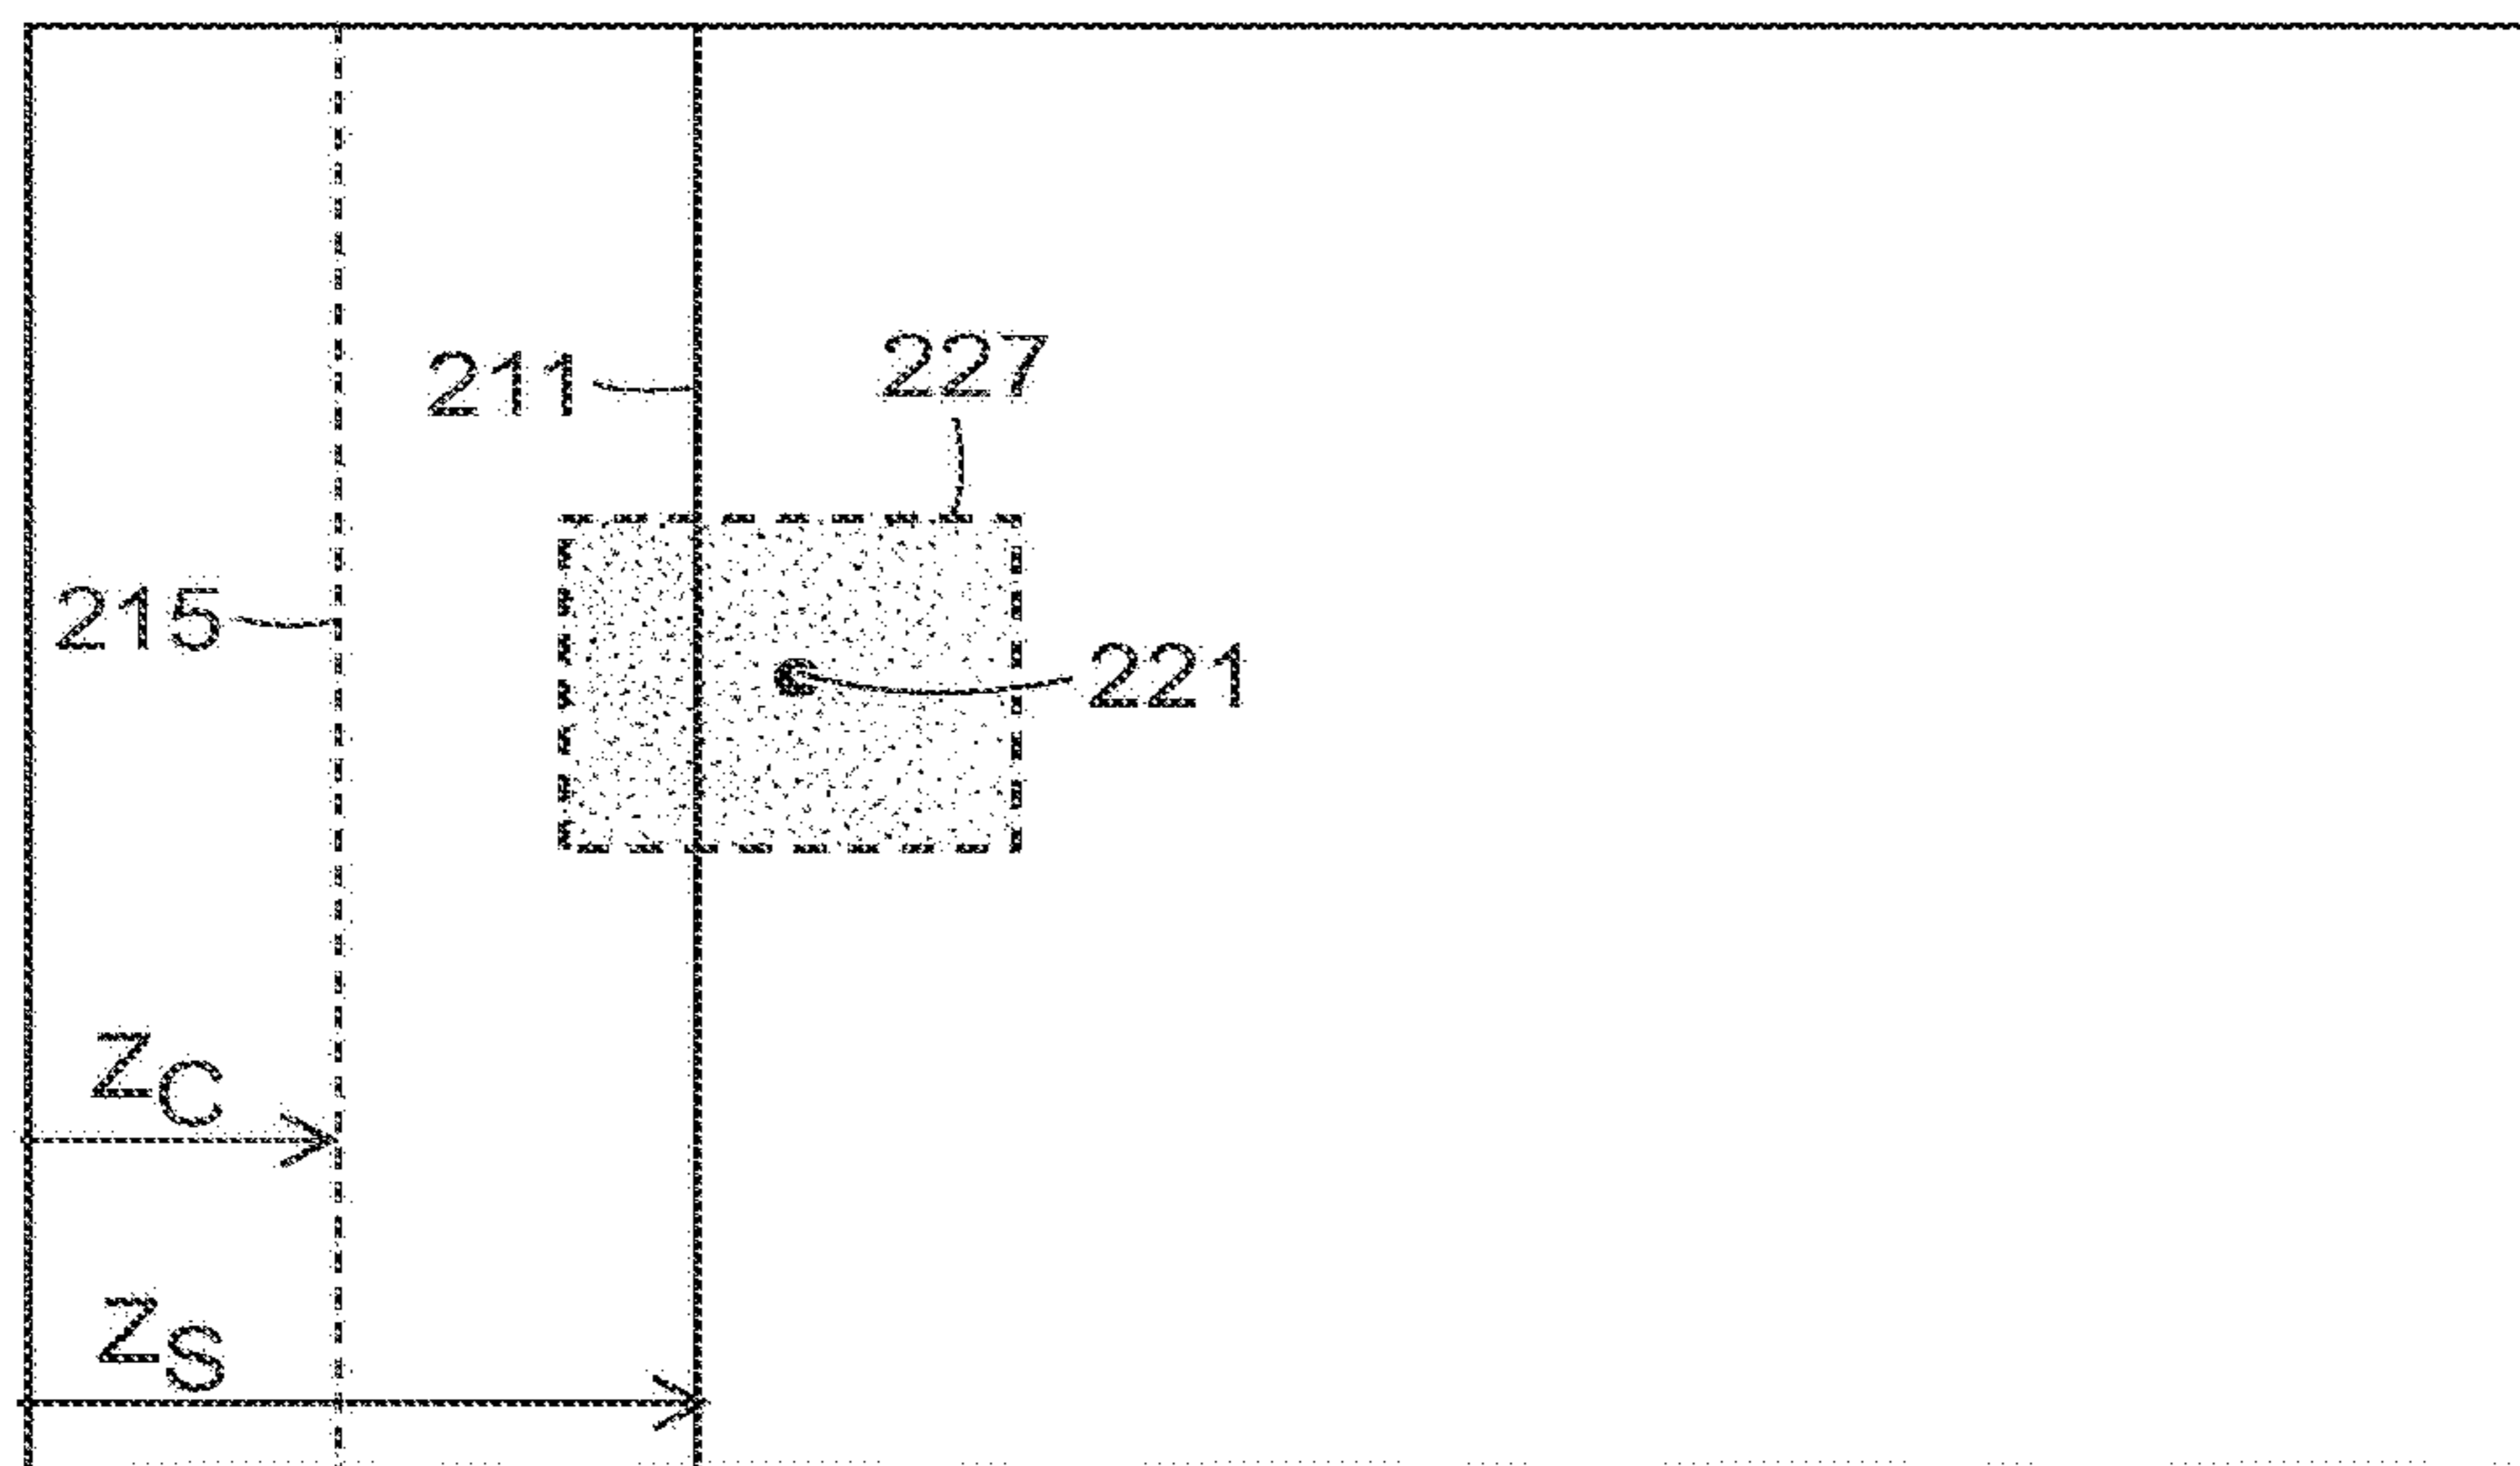


FIG. 20

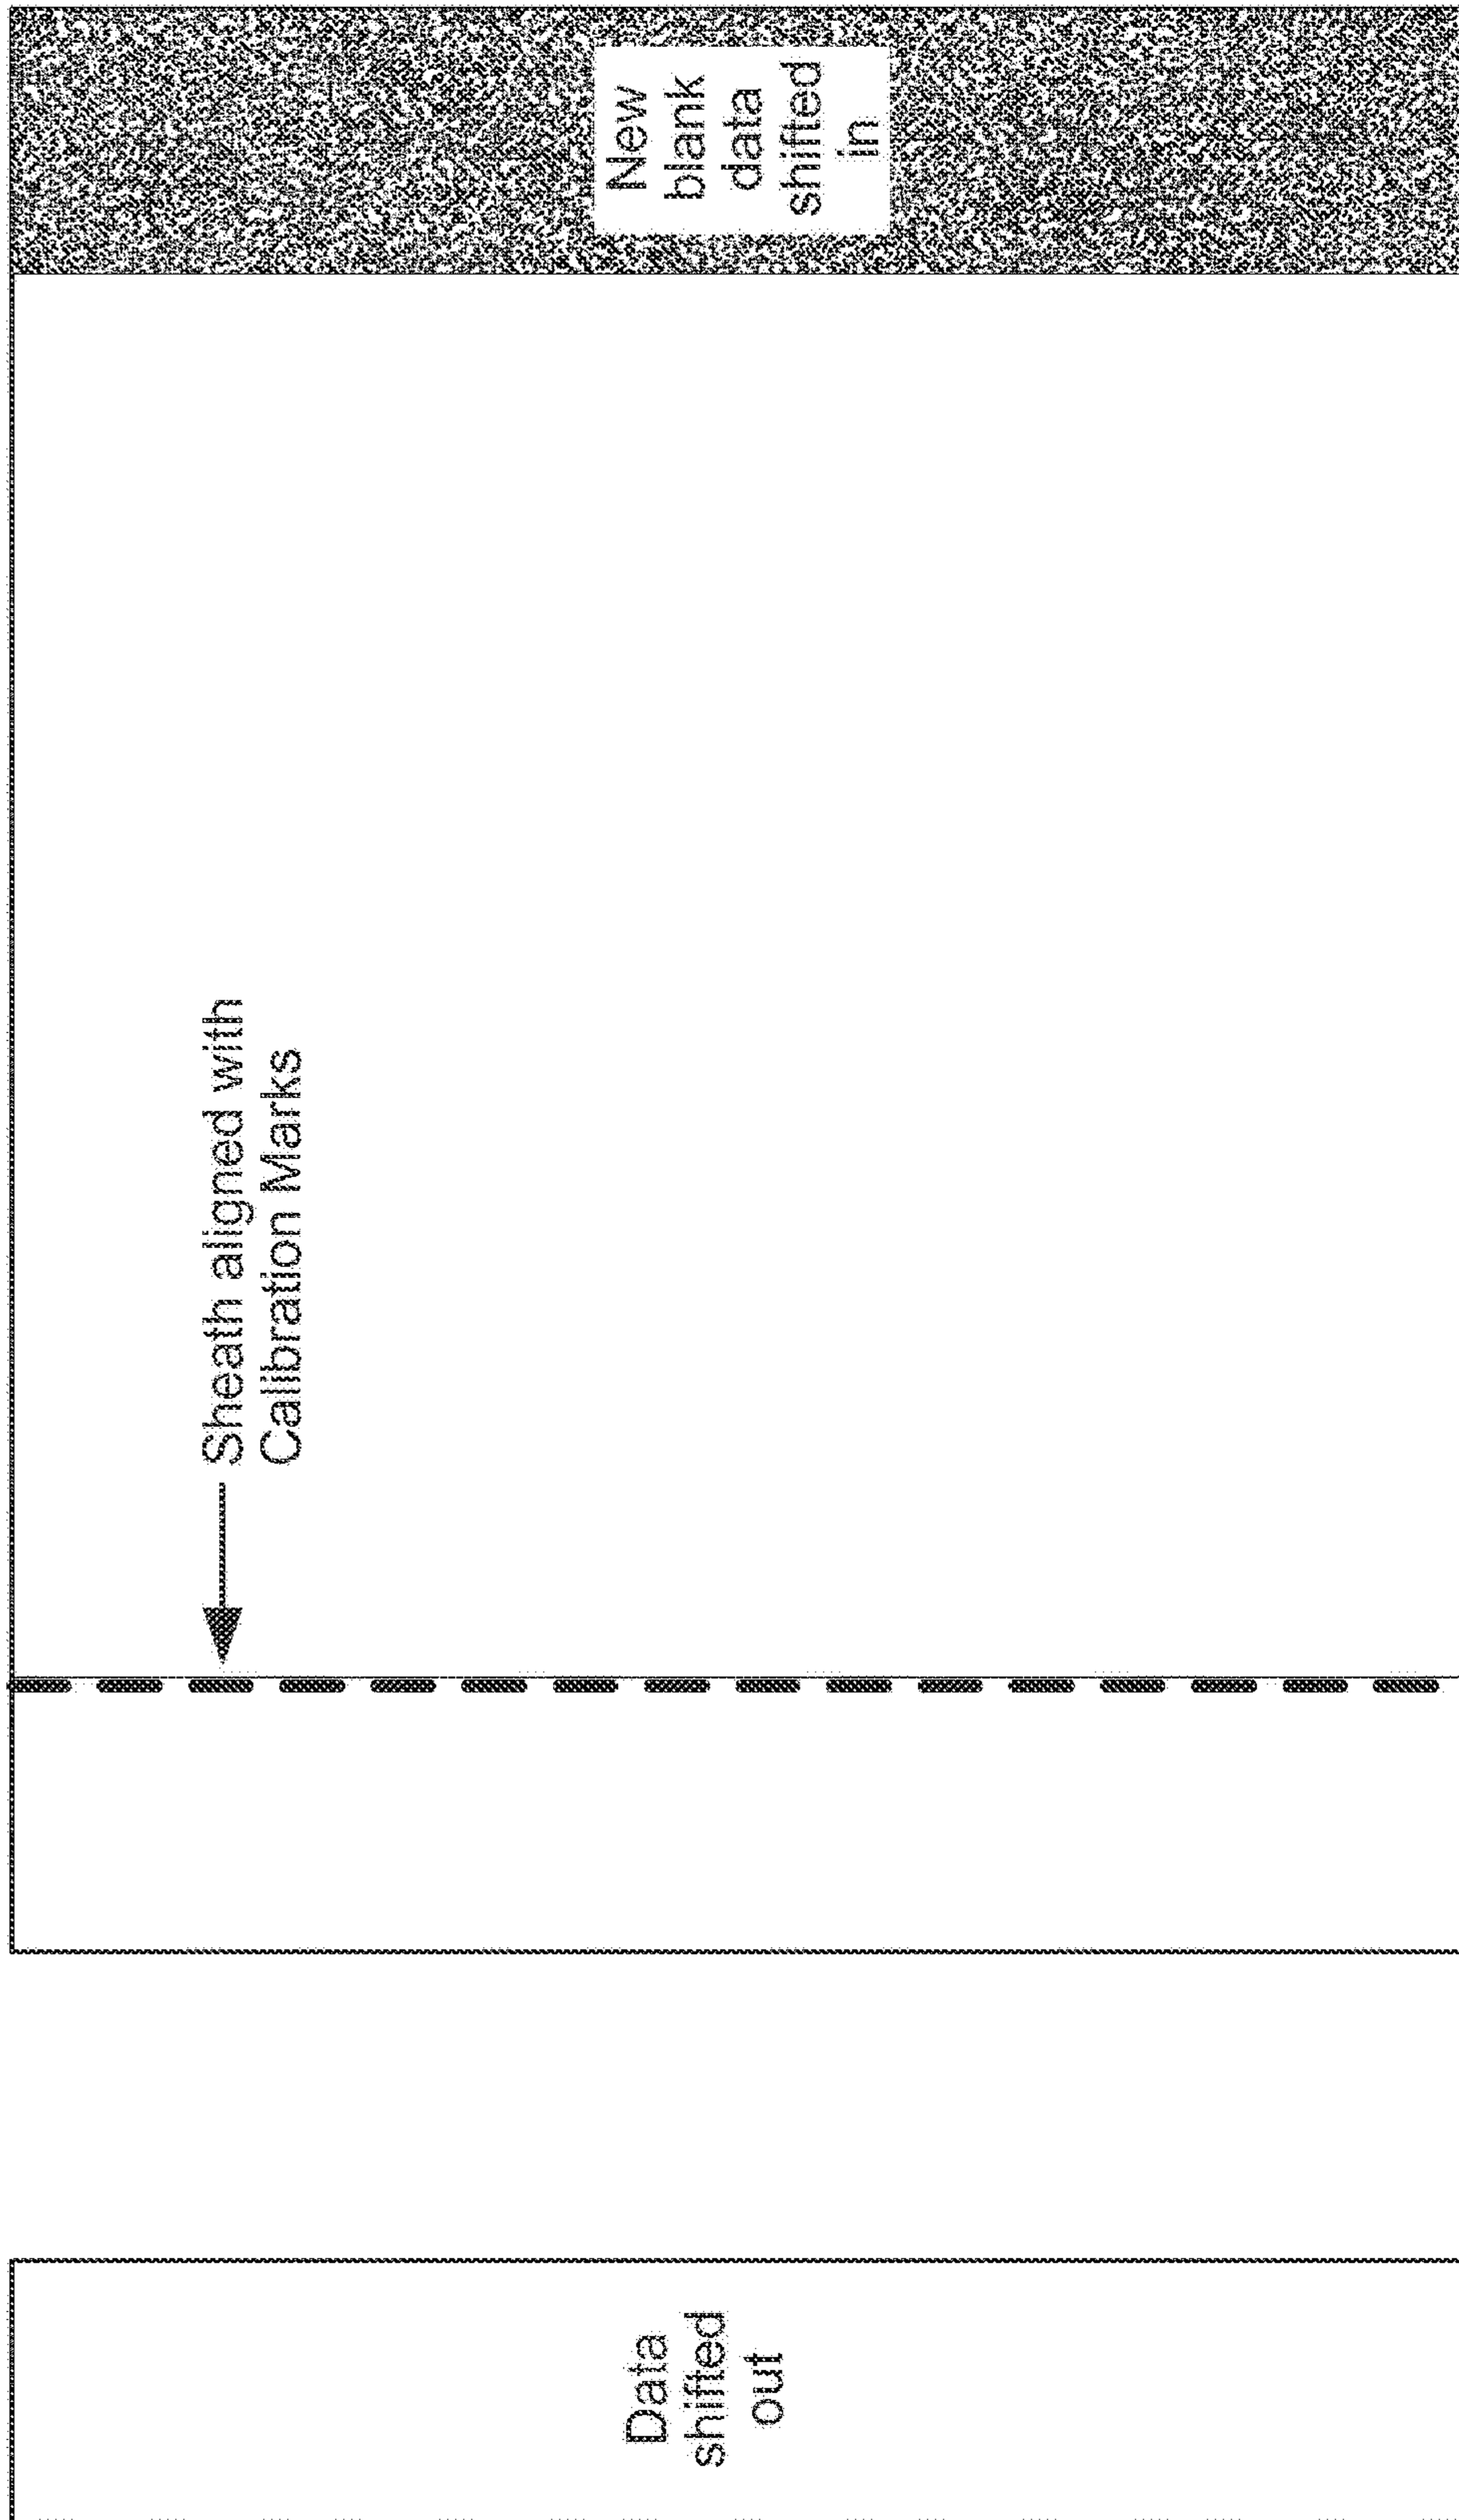


FIG. 21

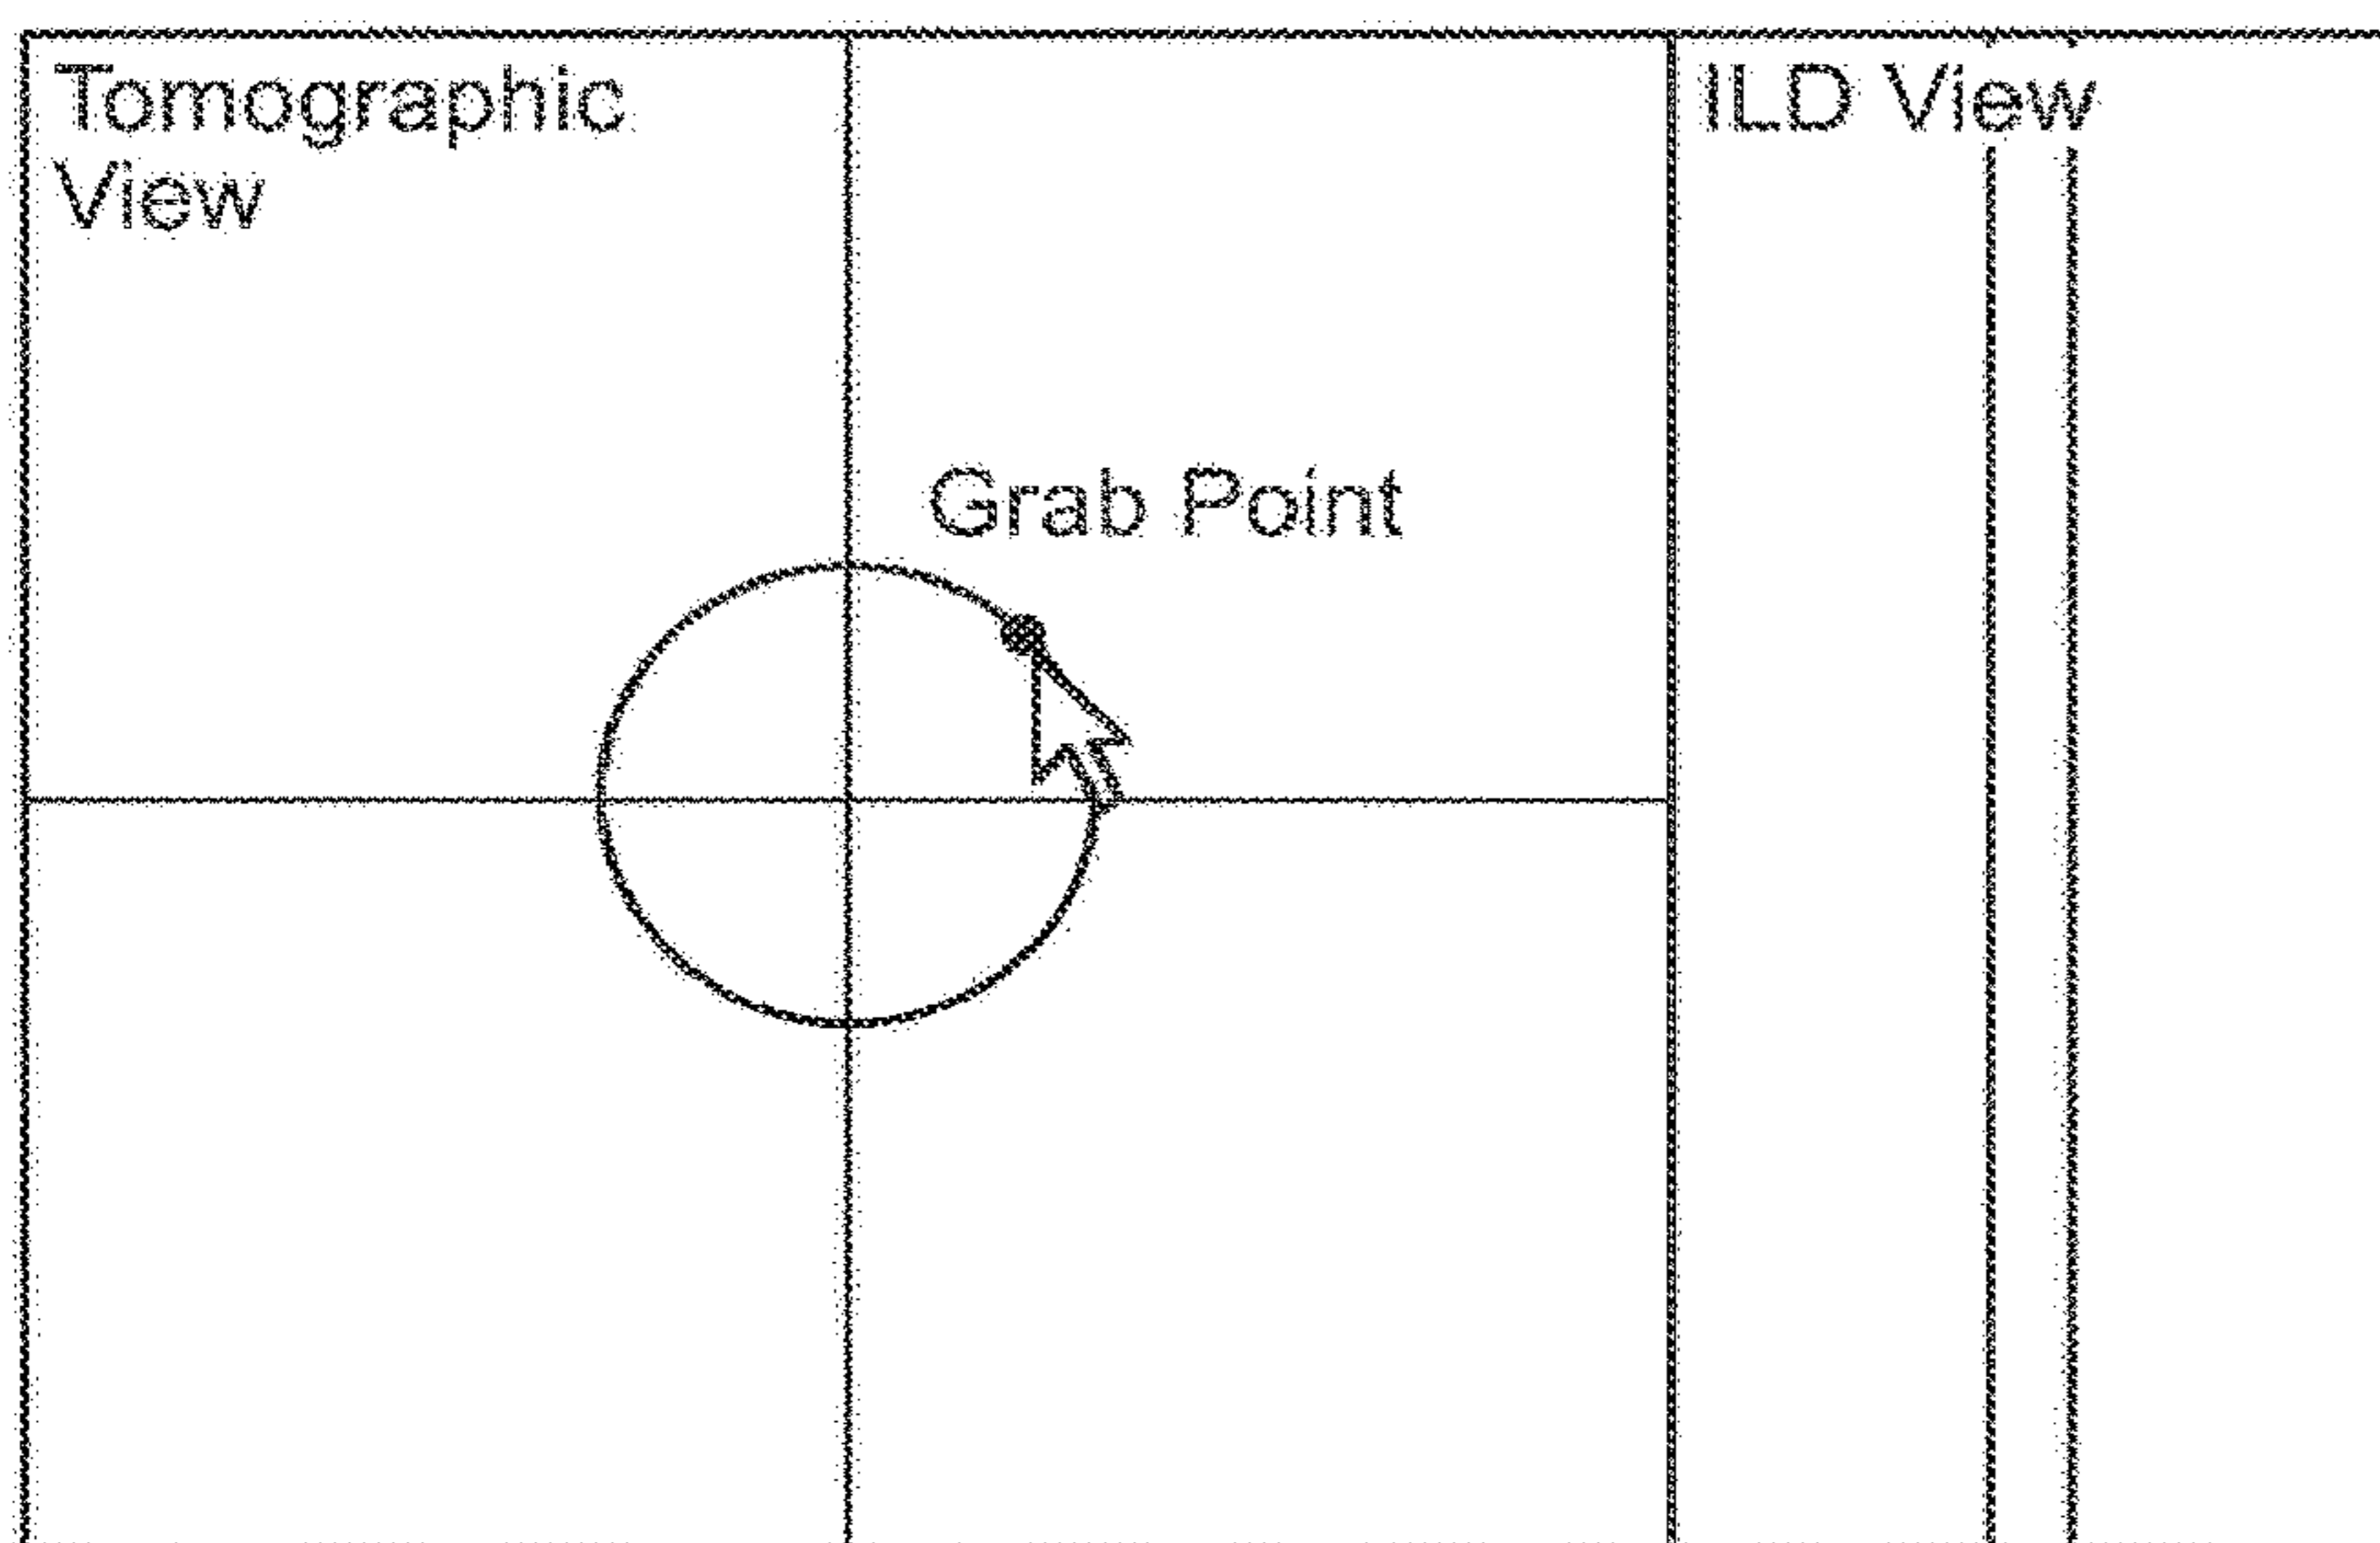


FIG. 22

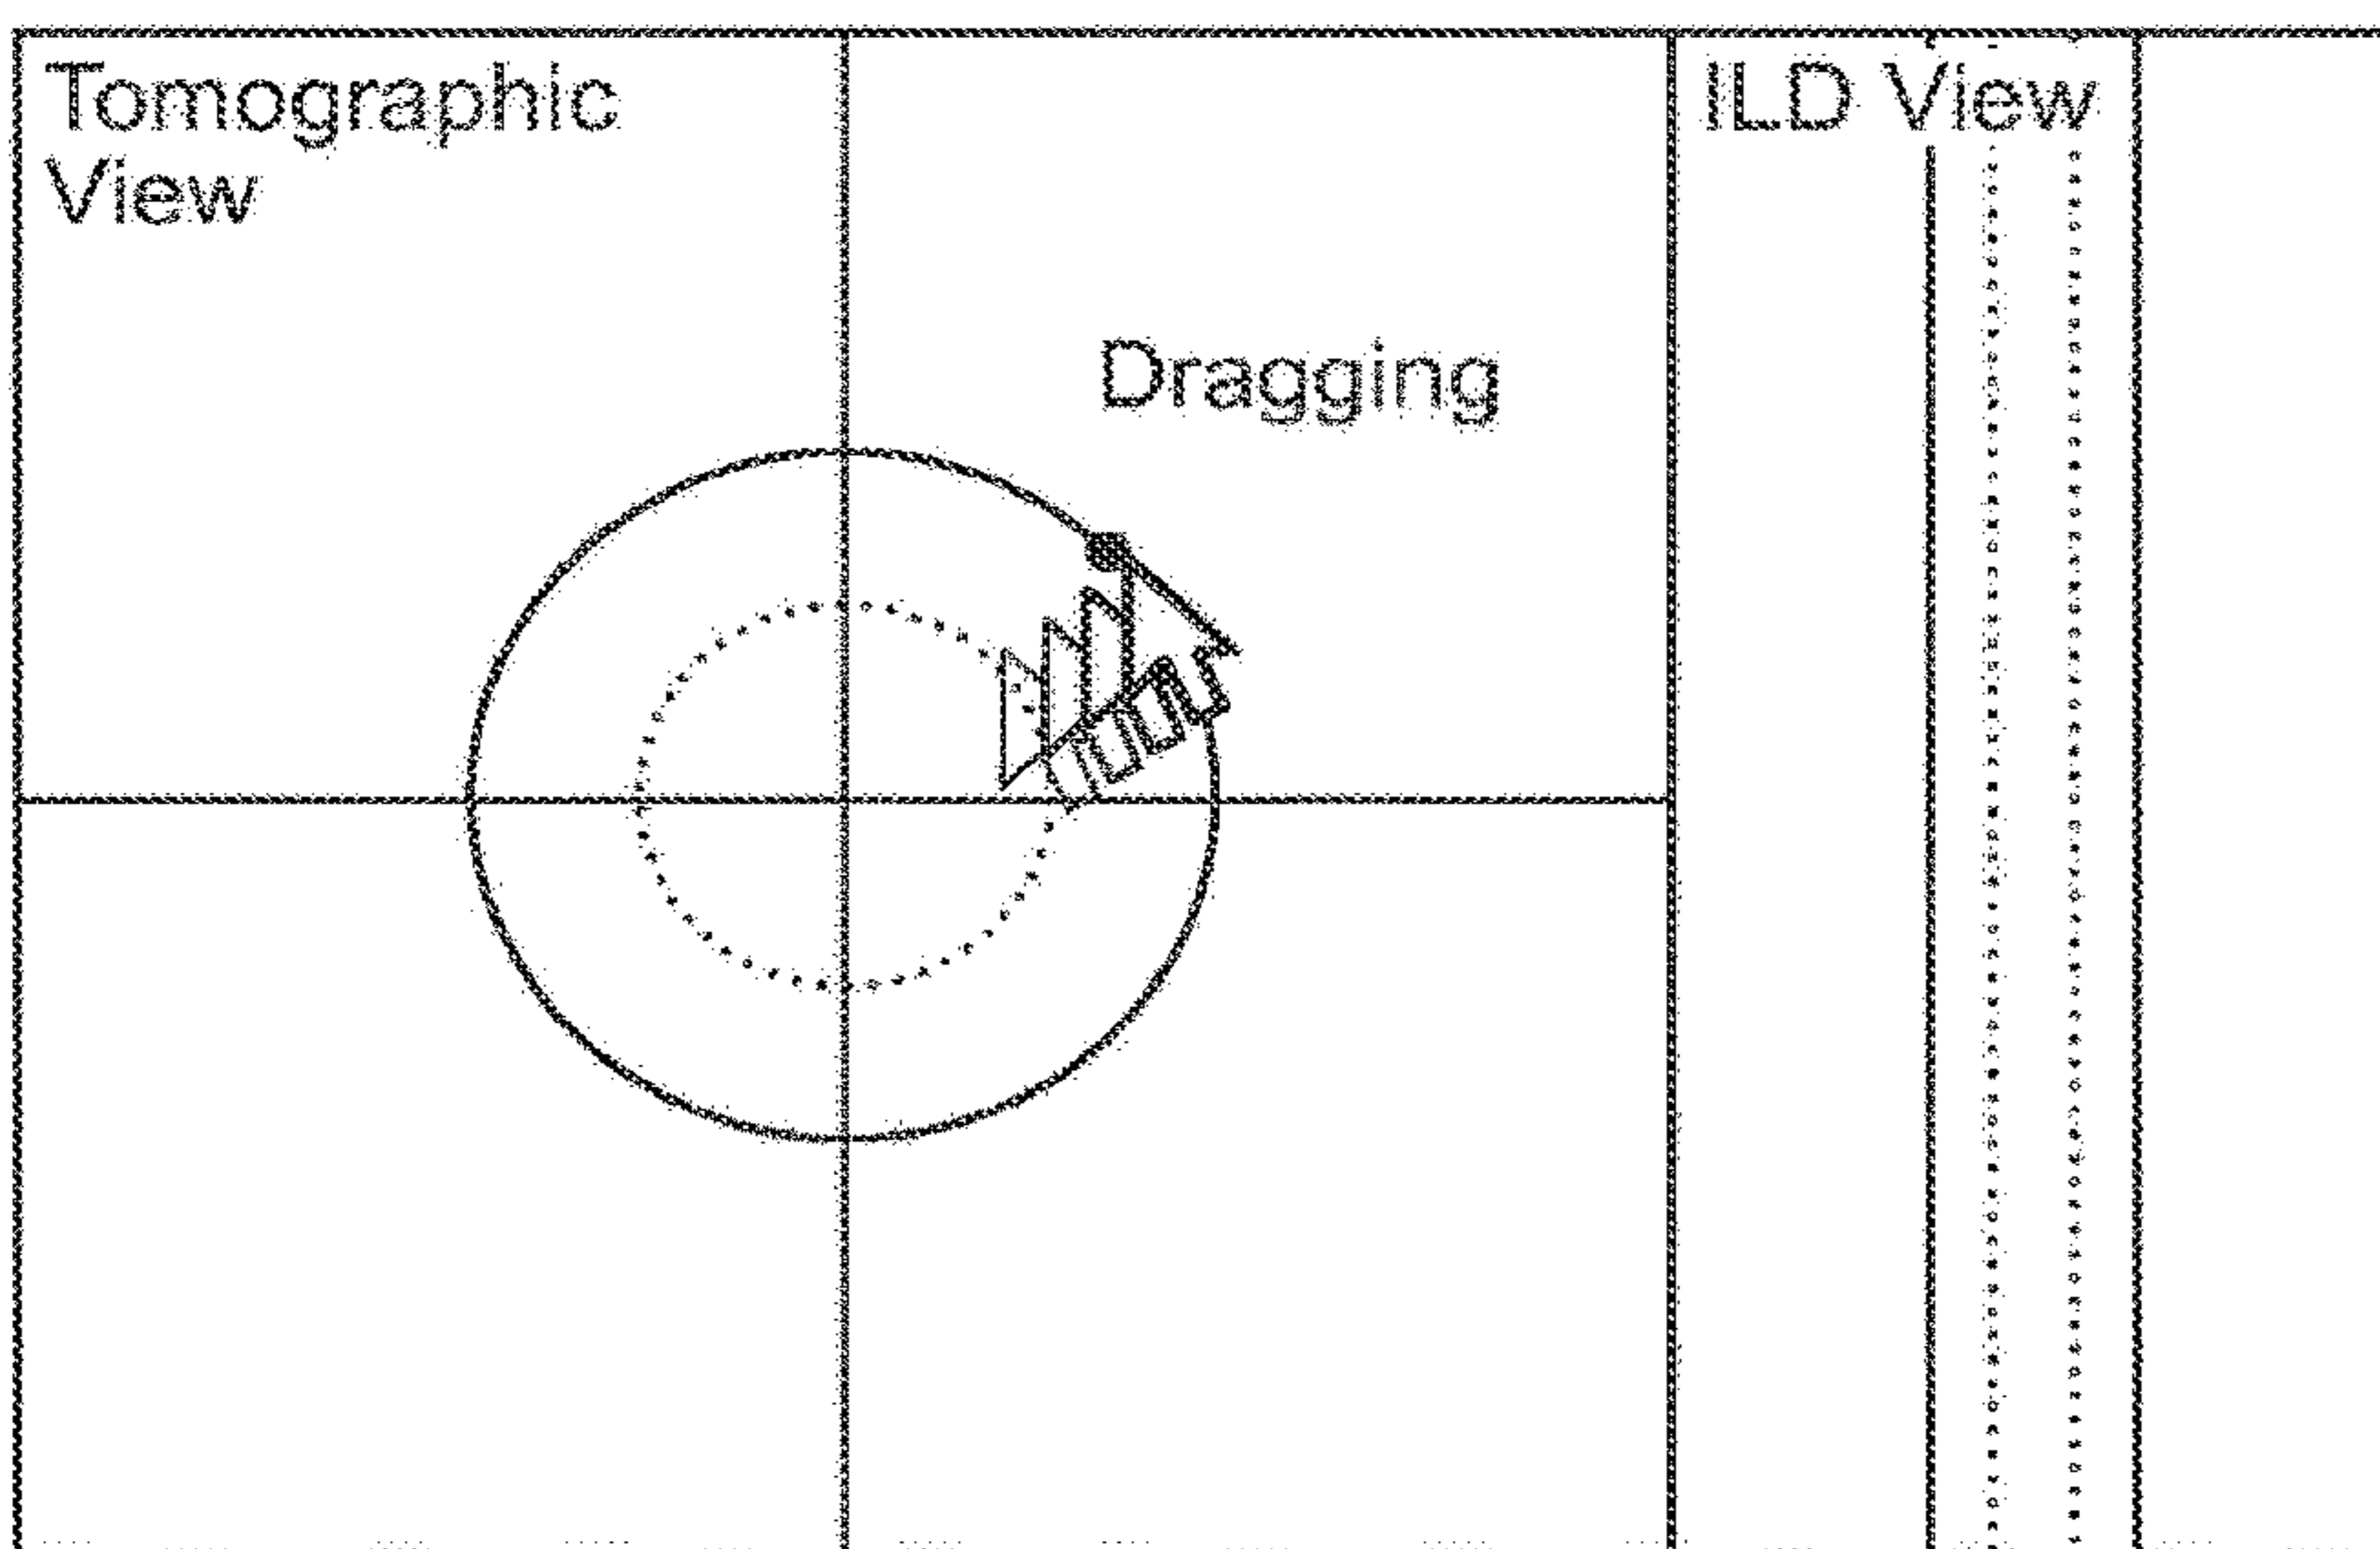


FIG. 23

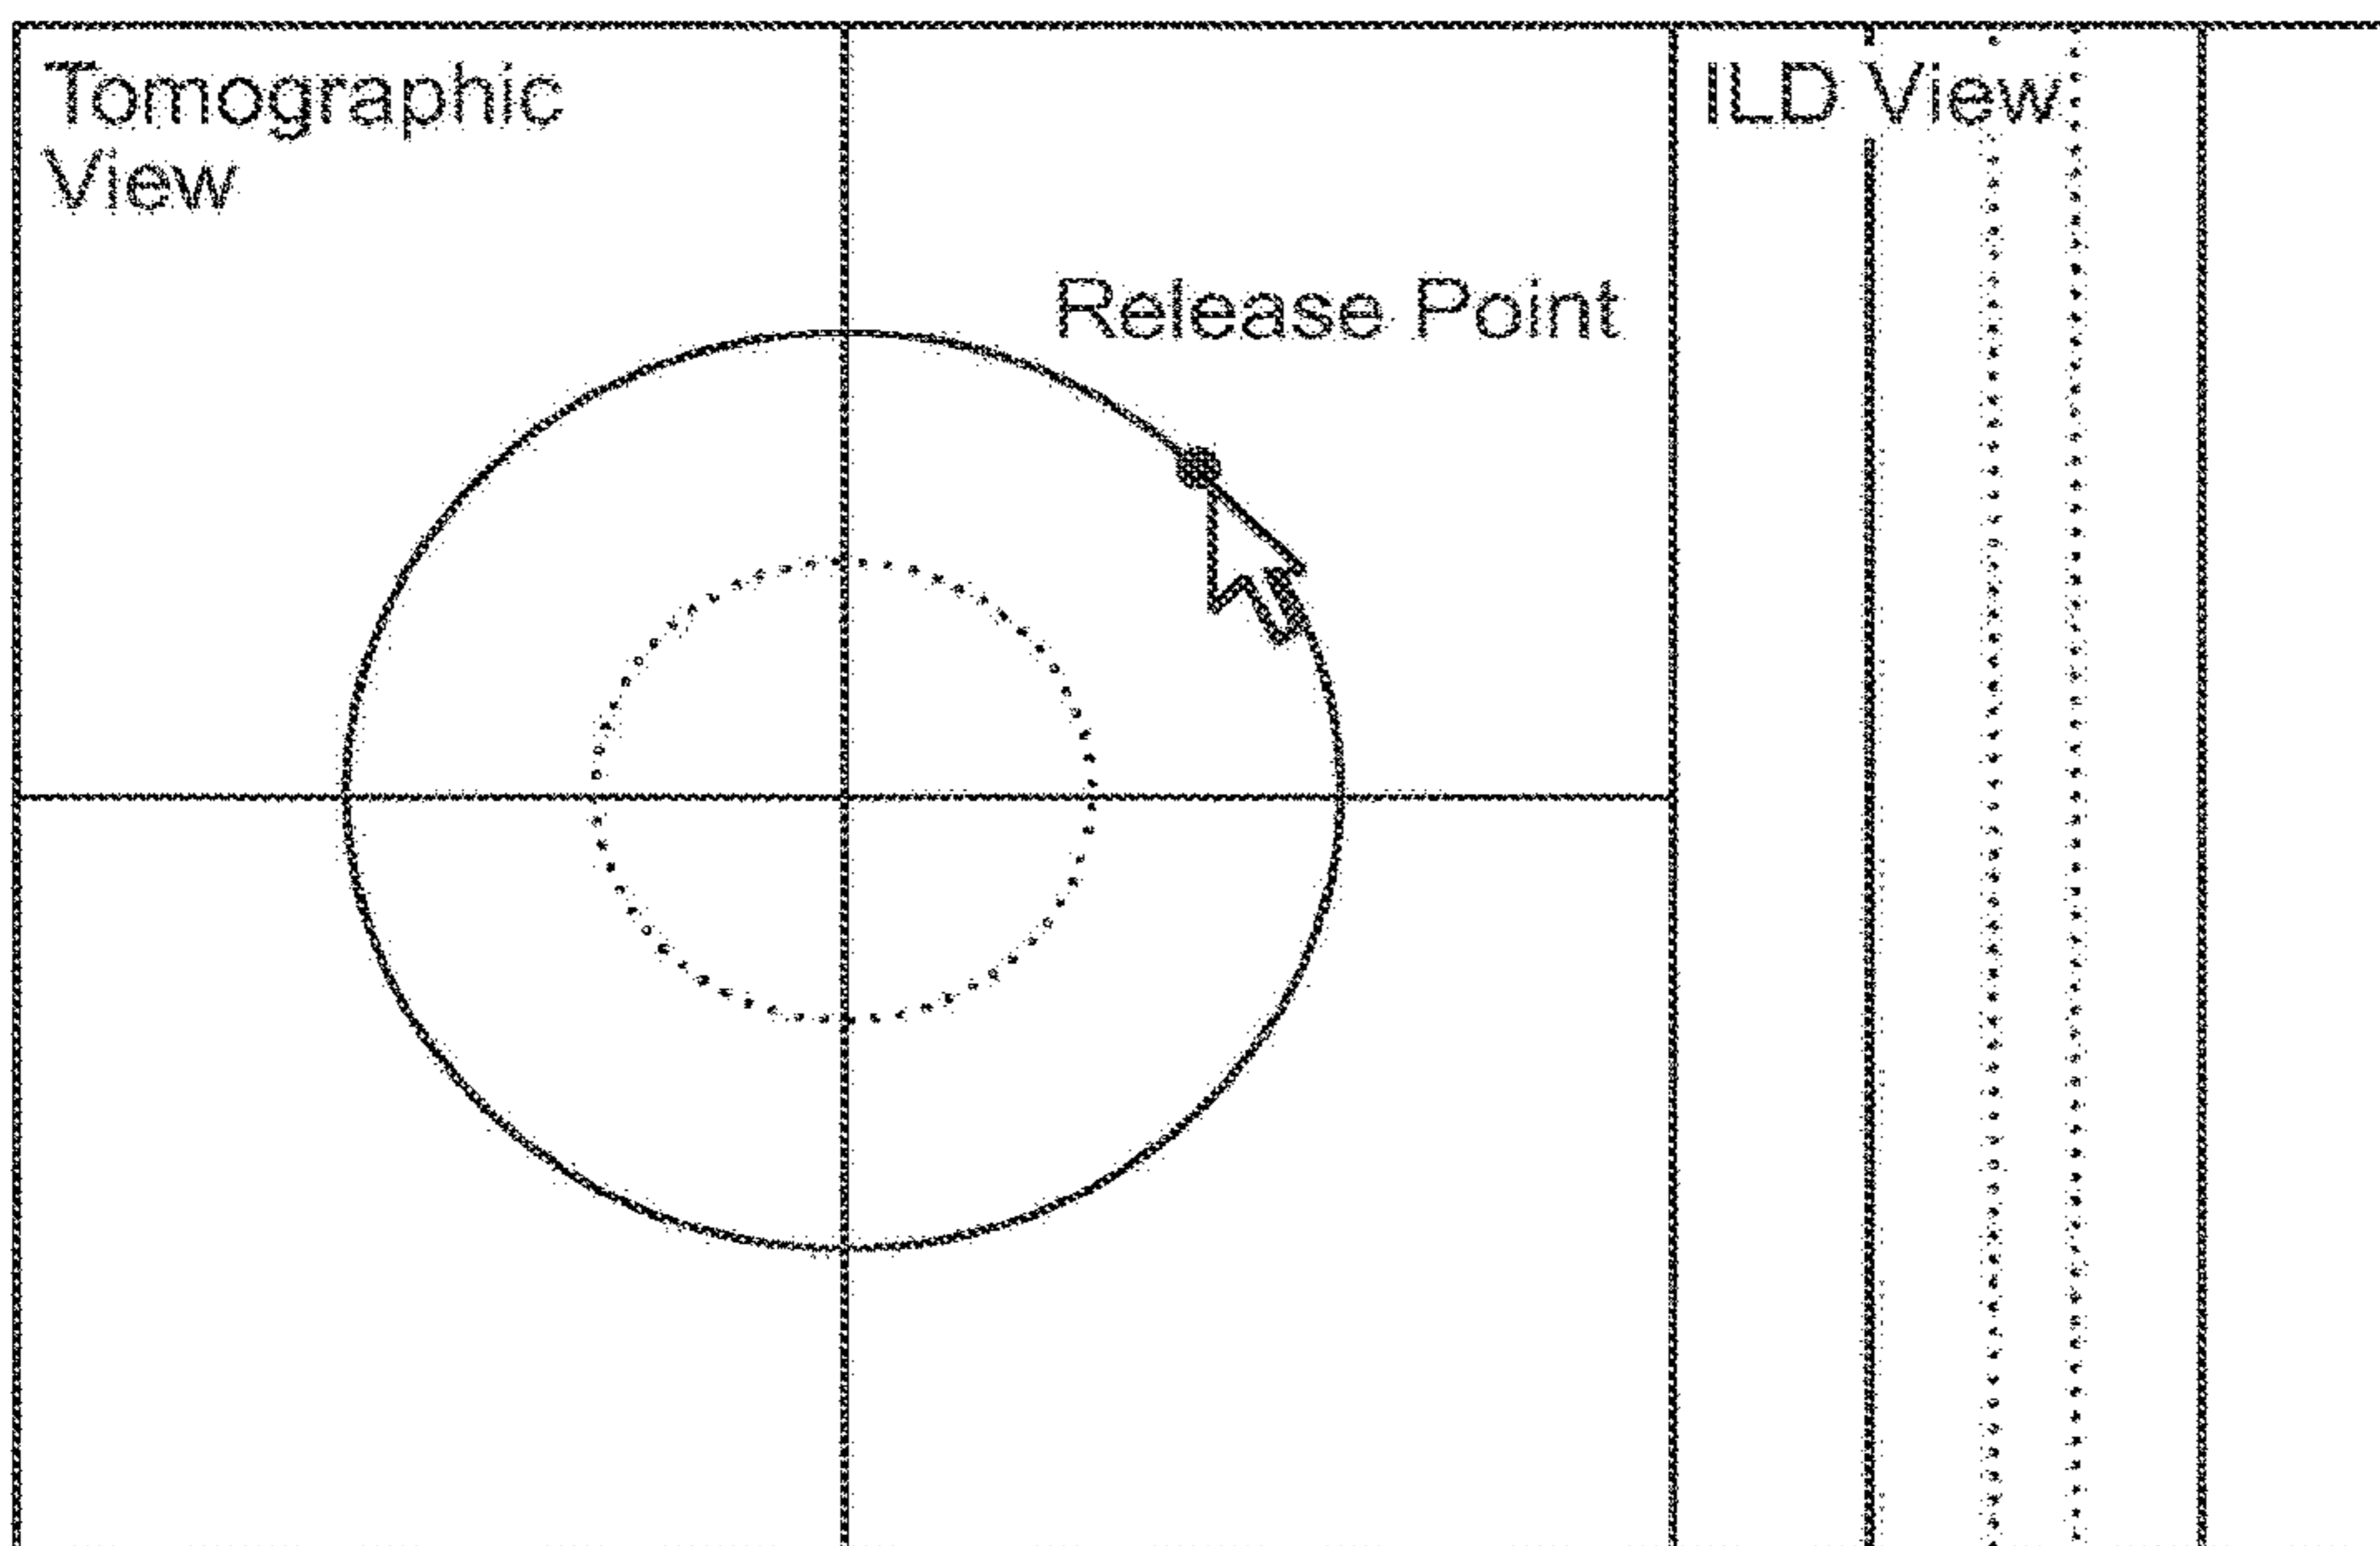


FIG. 24

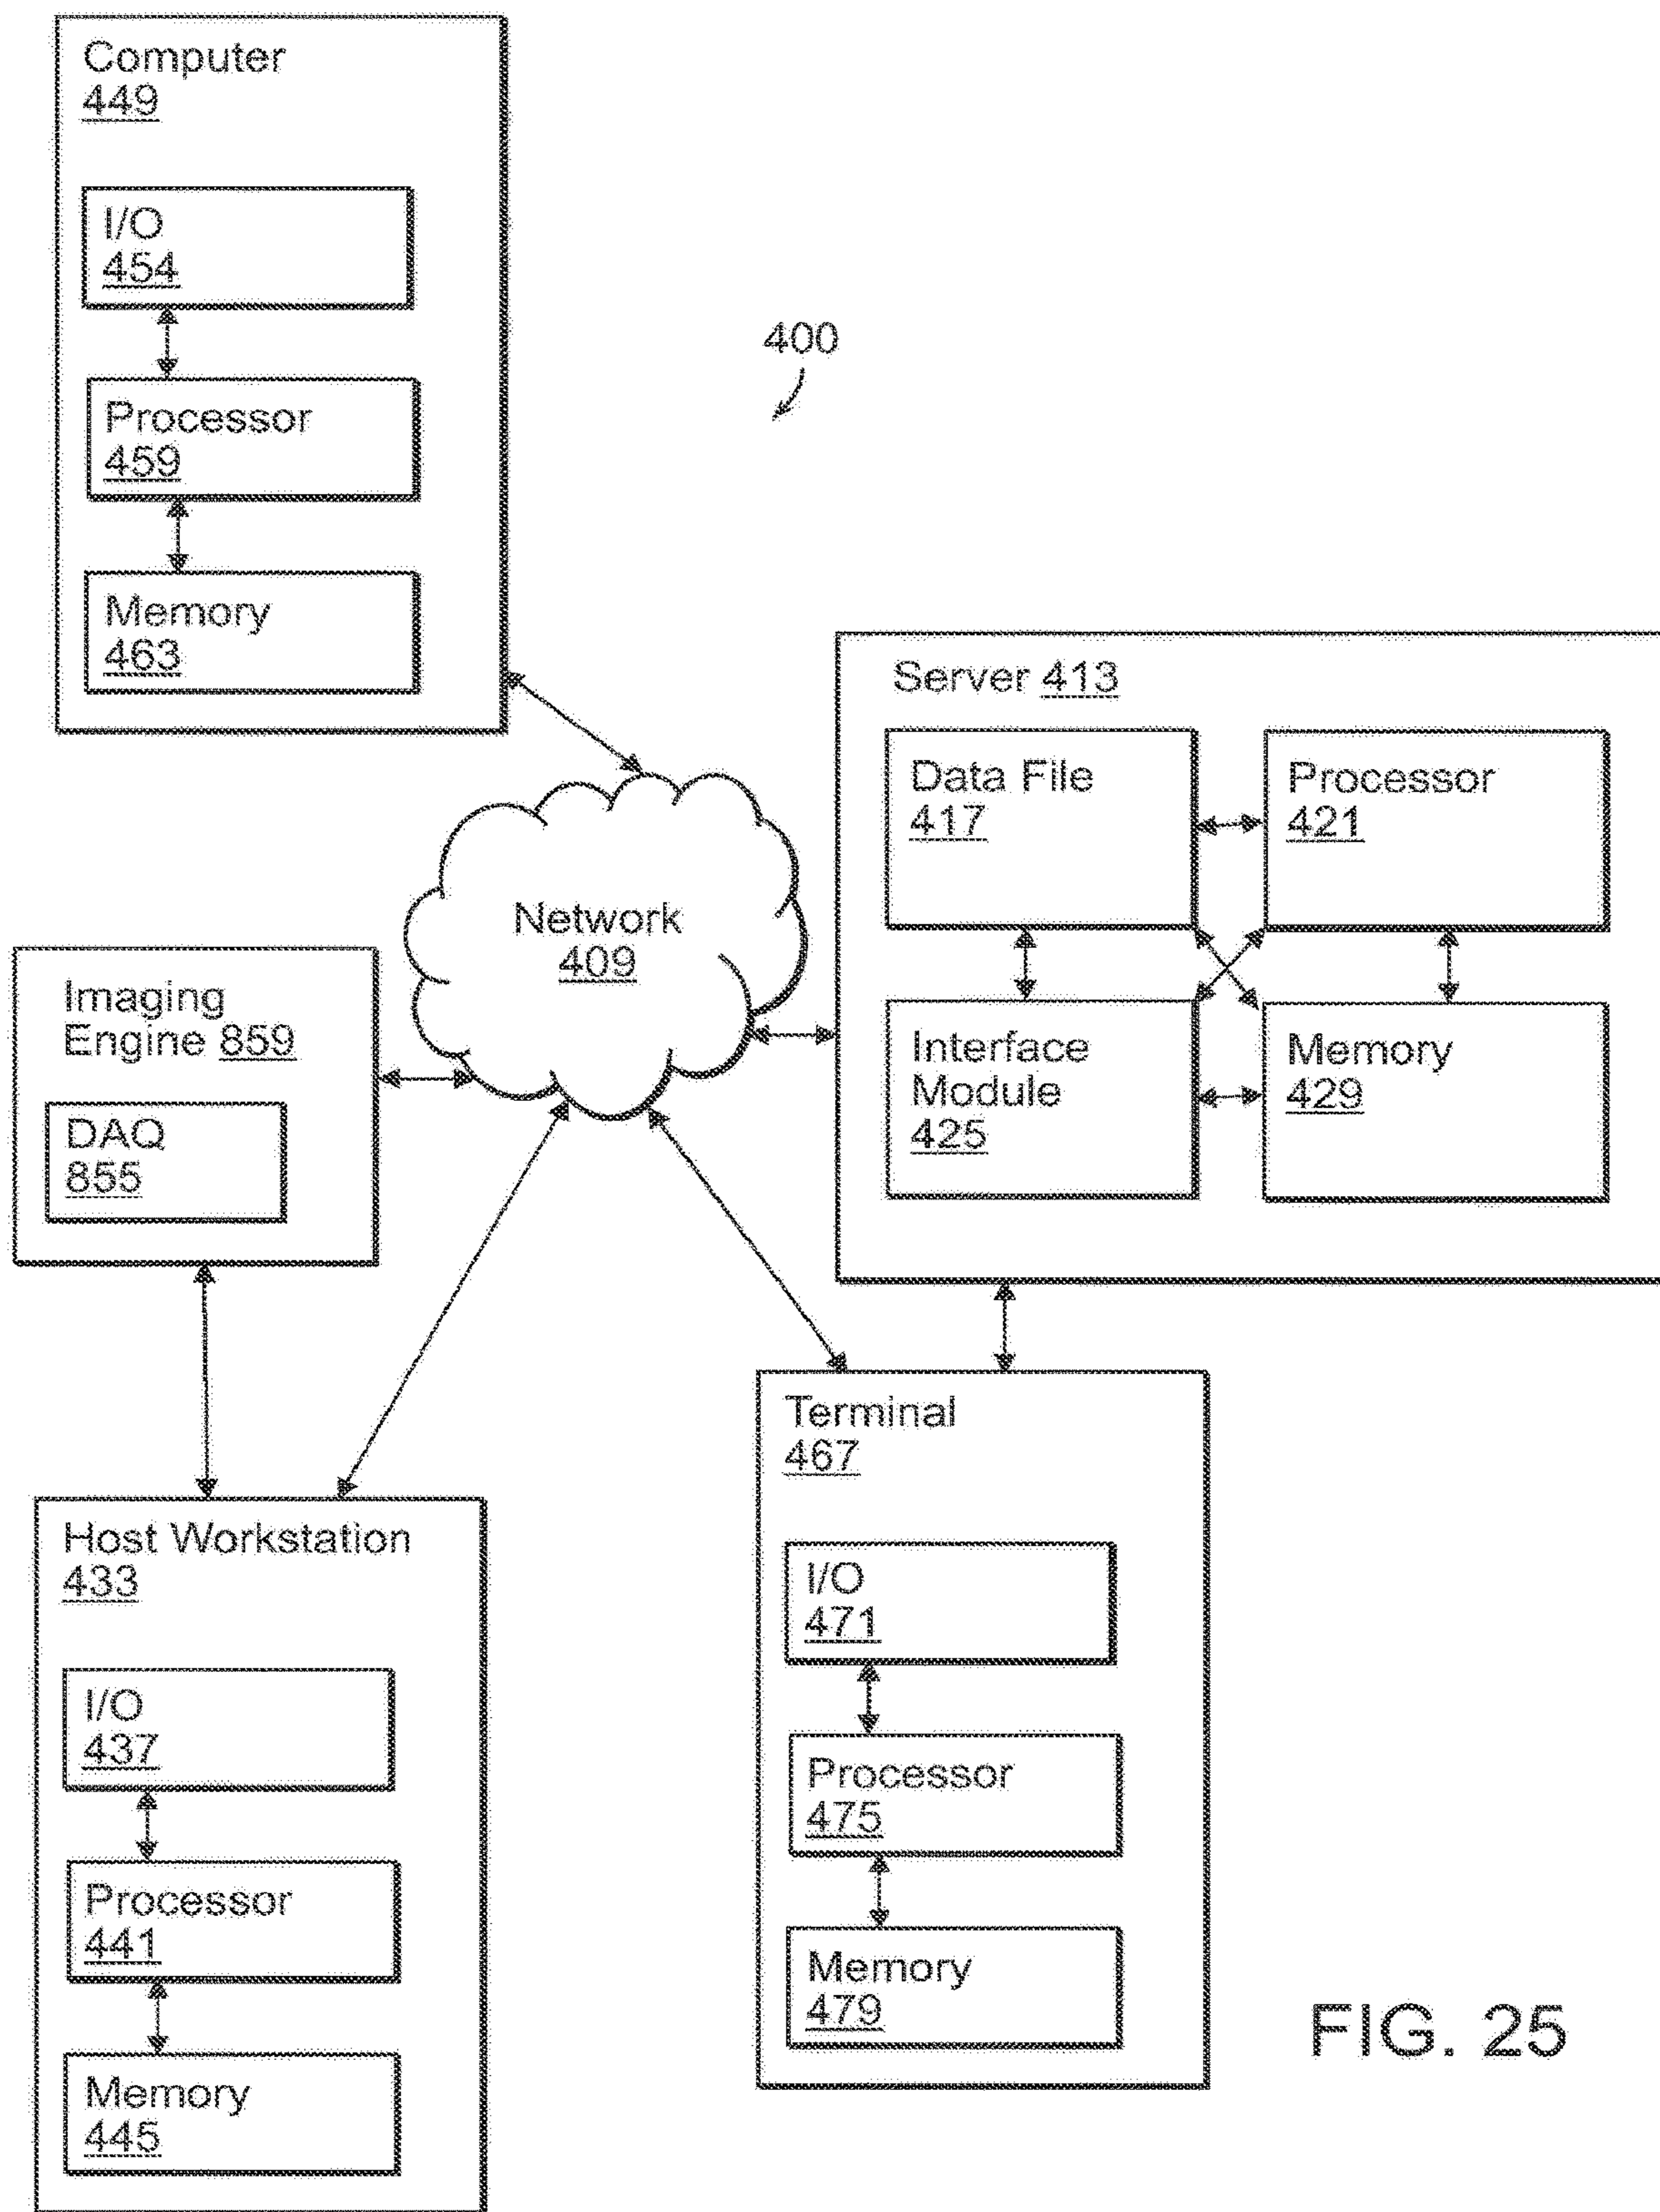


FIG. 25

MANUAL CALIBRATION OF IMAGING SYSTEM

RELATED APPLICATION

The present application is a continuation of U.S. patent application Ser. No. 14/107,861, filed Dec. 16, 2013, now U.S. Pat. No. 10,942,022, which claims the benefit of and priority to U.S. Provisional Application No. 61/739,881, filed Dec. 20, 2012, each of which is hereby incorporated by reference in its entirety.

TECHNICAL FIELD

The invention generally relates to methods for manually calibrating Time-of-Flight based imaging systems and interferometric systems more particularly, such as optical coherence tomography systems.

BACKGROUND

Time-of-Flight imaging technologies in medicine and other fields involve measuring the time required for light to travel from a light sources to a target and back to a detector. Those measurements are used to provide high resolution images of the target. Time-of-Flight principles have applications in such diverse technologies as optical coherence tomography (OCT), gated viewing, positron emission tomography (PET), and radiotherapy. Beyond medical imaging, time-of-flight technologies are used in computer vision, robotics, art restoration, laser speed enforcement, and vision aids with security and military applications.

One problem that arises in many time-of-flight measurement technologies relates to calibration. Light that has been sent and received by an imaging component such as a lens or a catheter can be used to present an image of the target. But, where a reference point or zero point is not known a priori, the image does not necessarily contain calibration information relating to scale. Different approaches to calibrating these systems have included automatic computer processing algorithms as well as iterative user manipulation.

Known computer processing algorithms are limited. Typical approaches involve programming a computer to try to identify a reference point of a known dimension in the image. But where the known reference point appears among other images with similar shapes or is partially obscured and appears incompletely, computer processors are not adept at the induction required to determine the location or extent of the reference point.

Manual calibration is limited by the imprecision of human input and the time required for multiple iterations of spotting a calibration target and inputting information then zooming, centering, or focusing and repeating the steps. In, for example, the medical imaging context, the time involved is problematic because calibration often must occur while the patient is being examined. The imprecision is problematic for at least two reasons. First, the system must be calibrated precisely so that the imaging operation can be focused on the intended target (i.e., scanning at the desired depth in OCT). Also, tissue conditions such as tumors, plaque, or glaucoma must be measured precisely to monitor the progress of the condition.

SUMMARY

The invention generally provides systems and methods for manually calibrating an imaging system in which a user

looks at an image of a target and indicates a point near a location of a reference point within the image. An image processing operation is employed to determine the precise location of the reference point. Thus, a user can identify the actual location of the reference point and a processing algorithm can give precision to the actual location. Where the reference point is, for example, a physical feature that gets imaged while the target is imaged, information about the expected location of that physical feature may be independently provided to the system. The system calculates a calibration value based on the expected and actual locations and adjusts to display an image at a known scale. Where the imaging system is operating live, it can take new images, providing them at the known scale. Where a user is reviewing stored images, the imaging system can adjust those stored images to provide them at a known scale. Because images are provided at a known scale, imaging systems can be focused on the intended target and the resulting images reveal dimensions of target subject matter. For example, in medical imaging, the dimensions of a feature within tissue can be measured to monitor the progress of a condition.

Systems and methods of the invention have particular utility in interferometric imaging applications where light from a reference path is combined with light from a sample path and the resulting interference pattern is analyzed. In OCT, for example, an interferometer is used to split light into fiber optic-based sample and reference paths. The length of the reference path must be adjusted to match the length of the sample path as defined by the outer surface of the imaging catheter sheath. The difference between the length of the sample and the reference path is the z-offset, which is zero when the paths have matched lengths. If the z-offset is known, the system can be calibrated by changing the length of the reference path to match the length of the sample path. This can be accomplished, for example, by operating a motor within a variable delay line (VDL) in the reference path. The invention provides methods for calibrating an interferometric imaging system by determining a z-offset of the system and using the determined z-offset value to provide an image at a known scale.

In certain aspects, the invention provides a method of calibrating an imaging system by displaying an image showing a target and a reference item, receiving user input indicating a point within the image, and detecting a location of the reference item within an area around the indicated point. If the reference is not detected within the area, the area may be expanded and the detection step repeated. The detected location is used to calculate a calibration value and a calibrated image of the target at a known scale is provided.

In some embodiments, the imaging system is an optical coherence tomography system. The reference item can be an image of a catheter sheath (e.g., a known surface such as the outer surface of the sheath). A scan from the system can be displayed, for example, on a computer monitor in tomographic view or in an image-longitudinal display. A user of the system can identify the catheter sheath and indicate its location by an input gesture, such as clicking with a mouse or touching a touchscreen. The reference item can be detected by a morphological image processing operation such as, for example, erosion, dilation, or a combination thereof. Where the imaging system is an intravascular OCT system, the catheter sheath may appear generally as a vertical lineal element in a B-scan.

A processor can begin by analyzing, for example, an area of the B-scan around a point corresponding to the user's input. Thus the user input is taken as a starting point, and image processing is performed to identify the reference item

(catheter sheath) within the area around the point. Using signal processing operations, the processing system finds a line in the area, for example, the highest valued contiguous line. The processing system can extrapolate and expand a search or processing algorithm. For example, where the line is substantially vertical, the system looks up and down to identify a location of substantially all of the catheter sheath.

In some OCT operations, an imaging catheter is associated with a specific sample path length. Path length may be provided with each catheter, for example, by a manufacturer. The catheter sample path length can give an expected location of the reference point. Where the expected location is thus provided, a difference between the actual location and the expected location can be used to detect and correct for, for example, path length changes (e.g., stretching) during operation.

With a calibration value calculated, the imaging system can provide a calibrated image—either in live mode, by making a new scan, or in review mode, by transforming stored image data.

In related aspects, the invention provides an imaging system that includes a processor and a computer-readable storage medium having instructions therein which can be executed to cause the system to display an image showing a target and a reference item, receive user input indicating a point within the image, and detect a location of the reference item within an area around the indicated point. The system uses the detected location to calculate a calibration value and provide a calibrated image of the target at a known scale.

In other aspects, the invention provides a method of calibrating an imaging system by displaying an image showing a target and a reference item, receiving user input indicating a motion of the reference item within the image, and calculating a calibration value based on indicated motion of the reference item. For example, a user can use a mouse to drag an image of the reference item onto a calibration mark, as seen on a computer screen. The user input indicating a motion of the reference item can be a drag-and-drop operation performed with a computer pointing device (e.g., mouse or trackpad), a drag along a touch-screen, or any other suitable computer input method. The motion indicated by the input is used to calculate the calibration value. Based on the calculated calibration value, a scaled image of the target is provided.

Methods of the invention include transforming the reference item within the image by, for example, re-sizing, rotation, translating, or a combination thereof. In some embodiments, the system is an interferometric imaging system and the reference item is a portion of the system itself. For example, where the reference item is an image of an OCT catheter sheath, the dragging motion can indicate a z-offset calibration value, i.e., a change in a radius associated with a zero-point in the image. The z-offset calibration can be accomplished by moving a VDL motor or transforming image data.

In some embodiments, the user input is received, and then the calibration operation (e.g., moving the VDL or transforming an existing image) is performed. In certain embodiments, the calibration operation is performed while the user input is received. Thus the user experiences that they are changing the image. Where an OCT system is used, the user experiences dragging the catheter sheath inwards or outwards (for example, to a reference calibration mark) and thus changing the image.

In some related aspects, the invention provides an imaging system that includes a processor and a computer-readable storage medium having instructions therein which can

be executed to cause the system to display an image showing a target and a reference item, receive user input indicating a motion of the reference item within the image, and calculate a calibration value based on indicated motion of the reference item. The calibration value is used to provide a scaled image of the target.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows use of an imaging system according to certain embodiments.

FIG. 2 is a diagram of components of an OCT system.

FIG. 3 diagrams components within a patient interface module (PIM).

FIG. 4 shows the structure of a PIM according to certain embodiments.

FIG. 5 is a diagram of components in an imaging engine.

FIG. 6 is a diagram of an interferometer for use with systems of certain embodiments.

FIGS. 7A and 7B illustrate a segment of a blood vessel.

FIG. 8 shows the motion of parts of an imaging catheter according to certain embodiments of the invention.

FIG. 9 shows an array of A scan lines of a three-dimensional imaging system according to certain embodiments of the invention.

FIG. 10 shows the positioning of A scans within a vessel.

FIG. 11 shows a B-scan.

FIG. 12 shows a tomographic view based on the B-scan of FIG. 10.

FIG. 13 illustrates a set of A scans used to compose a tomographic view.

FIG. 14 shows the set of A scans shown in FIG. 13 within a cross section of a vessel.

FIG. 15 shows a longitudinal plane through a vessel including several A scans.

FIG. 16 is a perspective view of an image longitudinal display (ILD) in the same perspective as the longitudinal plane shown in FIG. 15.

FIG. 17 shows a display of a system of the invention.

FIG. 18 is a display providing an image of the vessel shown in FIGS. 7A and 7B.

FIG. 19 illustrates receiving user input indicating a point within an image.

FIG. 20 shows an area around a point to be searched.

FIG. 21 shows a calibrated B-scan.

FIGS. 22 and 23 illustrates receiving user input indicating a motion

FIG. 24 illustrates providing a scaled image based on an indicated motion.

FIG. 25 illustrates components of a system according to certain embodiments of the invention.

DETAILED DESCRIPTION

The invention provides systems and methods for calibrating an imaging system. Systems and methods of the invention have application in imaging systems that require calibration to provide a scale. Exemplary systems include imaging and sensing systems based on principles of time-of-flight or coherent interference. In some embodiments, systems and applications contemplated for use with the invention include optical coherence tomography (OCT), time-of-flight cameras such as the CamCube 3.0 TOF camera sold under the trademark PDM[VISION] by PMD Technologies GmbH (Siegen, Germany), or time-of-flight positron emission tomography (PET) technologies. See, e.g., Placht et al., 2012, Fast time-of-flight camera based surface

registration for radiotherapy patient positioning, *Med Phys* 39:4-17; Karp et al., 2009, The benefit of time-of-flight in PET imaging, *J Nucl Med* 49:462-470. Other imaging systems for use with the invention include, for example, gated viewing, radiotherapy, intra-vascular ultrasound, mag-

netic resonance imaging, elastographic techniques such as magnetic resonance elastography or transient elastography systems such as FibroScan by Echosens (Paris, France), and electrical impedance tomography, as well as other applica-
 5 tions in computer vision, robotics, art restoration, laser speed enforcement, and vision aids with security and mili-
 10 tary applications.

In OCT systems, a light source is used to provide a beam of coherent light. The light source can include an optical gain medium (e.g., laser or optical amplifier) to produce
 15 coherent light by stimulated emission. In some embodiments, the gain medium is provided by a semiconductor optical amplifier. A light source may further include other components, such as a tunable filter that allows a user to select a wavelength of light to be amplified. Wavelengths
 20 commonly used in medical applications include near-infrared light, for example between about 800 nm and about 1700 nm.

Generally, there are two types of OCT systems, common beam path systems and differential beam path systems, that differ from each other based upon the optical layout of the systems. A common beam path system sends all produced light through a single optical fiber to generate a reference signal and a sample signal whereas a differential beam path system splits the produced light such that a portion of the light is directed to the sample and the other portion is directed to a reference surface. Common beam path systems are further described for example in U.S. Pat. Nos. 7,999, 938; 7,995,210; and 7,787,127 the contents of each of which are incorporated by reference herein in their entirety.
 25

In a differential beam path system, the coherent light from the light source is input into an interferometer and split into a reference path and a sample path. The sample path is directed to the target and used to image the target. Reflections from the sample path are joined with the reference path and the combination of the reference-path light and the sample-path light produces interference patterns in the resulting light. The light, and thus the patterns, are converted to electric signals, which are then analyzed to produce depth-resolved images of the target tissue on a micron scale. Exemplary differential beam path interferometers are Mach-Zehnder interferometers and Michelson interferometers. Differential beam path interferometers are further described for example in U.S. Pat. Nos. 7,783,337; 6,134,003; and 6,421,164, the contents of each of which are incorporated by
 35 reference herein in its entirety.

Commercially available OCT systems are employed in diverse applications, including art conservation and diagnostic medicine, notably in ophthalmology where OCT can be used to obtain detailed images from within the retina. The detailed images of the retina allow one to identify diseases and trauma of the eye. Other applications of imaging systems of the invention include, for example, dermatology (e.g., to image subsurface structural and blood flow formations), dentistry (to image teeth and gum line), gastroenterology (e.g., to image the gastrointestinal tract to detect polyps and inflammation), and cancer diagnostics (for example, to discriminate between malignant and normal tissue).

In certain embodiments, systems and methods of the invention image within a lumen of tissue. Various lumen of biological structures may be imaged including, for example,

blood vessels, including, but not limited, to vasculature of the lymphatic and nervous systems, various structures of the gastrointestinal tract including lumen of the small intestine, large intestine, stomach, esophagus, colon, pancreatic duct, bile duct, hepatic duct, lumen of the reproductive tract including the vas deferens, vagina, uterus and fallopian tubes, structures of the urinary tract including urinary collecting ducts, renal tubules, ureter, and bladder, and structures of the head and neck and pulmonary system including
 5 sinuses, parotid, trachea, bronchi, and lungs. Systems and methods of the invention have particular applicability in imaging veins and arteries such as, for example, the arteries of the heart. Since an OCT system can be calibrated to provide scale information, intravascular OCT imaging of the coronary arteries can reveal plaque build-up over time, change in dimensions of features, and progress of thrombotic elements. The accumulation of plaque within the artery wall over decades is the setup for vulnerable plaque which, in turn, leads to heart attack and stenosis (narrowing) of the artery. OCT images, if scaled or calibrated, are useful in determining both plaque volume within the wall of the artery and/or the degree of stenosis of the artery lumen. Intravascular OCT can also be used to assess the effects of treatments of stenosis such as with hydraulic angioplasty expansion of the artery, with or without stents, and the results of medical therapy over time.
 10
 15
 20
 25

FIG. 1 depicts the use of an exemplary intravascular OCT system 801. A physician controls an imaging catheter 826 through use of a handheld patient interface module (PIM) 839 to collect image data from a patient. Image data collected through catheter 826 is transmitted by PIM cable 841 to an imaging engine 859, which can be, for example, housed within a bedside unit or in a nearby computer installation or in a server rack coupled via networking technologies. As shown in FIG. 1, an OCT system can further include a workstation 433 (e.g., a monitor, keyboard, and mouse).
 30
 35

FIG. 2 gives a block diagram of components of OCT system 801. Imaging engine 859 is coupled to PIM 839 via PIM cable 841. Imaging catheter 826 extends from PIM 839 to the site of imaging. Engine cable 845 connects imaging engine 859 to host workstation 433. OCT is discussed in U.S. Pat. No. 8,108,030; U.S. Pub. 2011/0152771; U.S. Pub. 2010/0220334; U.S. Pub. 2009/0043191; U.S. Pub. 2008/0291463; and U.S. Pub. 2008/0180683, the contents of each of which are incorporated by reference in their entirety for all purposes. In certain embodiments, systems and methods of the invention include processing hardware configured to interact with more than one different three dimensional imaging system so that the tissue imaging devices and methods described here in can be alternatively used with OCT, IVUS, or other hardware.
 40
 45
 50

As shown in FIG. 1, an operator controls imaging catheter 826 via handheld PIM 839. PIM 839 may include controls such as knobs or buttons to start or stop operation, set or vary speed or displacement, or otherwise control the imaging operation. PIM 839 further includes hardware for operating the imaging catheter.

FIG. 3 shows components of PIM 839. Catheter 826 is mounted to PIM 839 via a catheter receptacle 869. Spin motor 861 is provided to rotate catheter 826 and pullback motor 865 is provided to drive lateral translation of catheter 826. Also depicted is a keypad for input/output, a fiber-optic rotary joint (iFORj), a printed circuit board assembly (PCBA), and optional RFID components.
 55
 60
 65

FIG. 4 gives a perspective view of PIM 839 with a keypad cover removed. Spin motor 861 is provided to rotate catheter

826 and pullback motor **865** causes lateral translation. Optical signals, electrical signals, or both arrive at PIM **839** via PIM cable **841**. PIM cable **841** extends to imaging engine **859** as shown in FIG. 2.

FIG. 5 shows components of imaging engine **859**. As shown in FIG. 5, the imaging engine **859** (e.g., a bedside unit) houses a power distribution board **849**, light source **827**, interferometer **831**, and variable delay line **835** as well as a data acquisition (DAQ) board **855** and optical controller board (OCB) **851**.

Light source **827**, as discussed above, may use a laser or an optical amplifier as a source of coherent light. Coherent light is transmitted to interferometer **831**.

FIG. 6 shows a path of light through interferometer **831** during OCT imaging. Coherent light for image capture originates within the light source **827**. This light is split between an OCT interferometer **905** and an auxiliary, or “clock”, interferometer **911**. Light directed to the OCT interferometer is further split by splitter **917** and recombined by splitter **919** with an asymmetric split ratio. The majority of the light is guided into the sample path **913** and the remainder into a reference path **915**. The sample path includes optical fibers running through the PIM **839** and the imaging catheter **826** and terminating at the distal end of the imaging catheter where the image is captured.

An image is captured by introducing imaging catheter **826** into a target within a patient, such as a lumen of a blood vessel. This can be accomplished by using standard interventional techniques and tools such as a guide wire, guide catheter, or angiography system. Suitable imaging catheters and their use are discussed in U.S. Pat. Nos. 8,116,605 and 7,711,413, the contents of which are incorporated by reference in their entirety for all purposes.

FIG. 7A provides an illustration of a segment of a vessel **101** having a feature **113** of interest. FIG. 7B shows a cross-section of vessel **101** through feature **113**. In certain embodiments, intravascular imaging involves positioning imaging catheter **826** within vessel **101** near feature **113** and collecting data to provide a three-dimensional image. Data can be collected in three dimensions by rotating catheter **826** around a catheter axis to collect image data in radial directions around the catheter while also translating catheter **826** along the catheter axis. As a result of combined rotation and translation, catheter **826** collects image data from a series of scan lines (each referred to as an A-scan line, or A-scan) disposed in a helical array.

FIG. 8 shows the motion of parts of an imaging catheter according to certain embodiments of the invention. Rotation of imaging catheter **826** around axis **117** is driven by spin motor **861** while translation along axis **117** is driven by pullback motor **865**, as discussed above with reference to FIG. 4. An imaging tip of catheter **826** generally follows helical trace **119**, resulting in a motion for image capture described by FIG. 8. Blood in the vessel is temporarily flushed with a clear solution for imaging. When operation is triggered from PIM **839** or a control console, the imaging core of catheter **826** rotates while collecting image data, which data is delivered to the imaging system.

FIG. 9 illustrates the helical array of A-scan lines $A_{11}, A_{12}, \dots, A_N$ captured by the imaging operation.

FIG. 10 is provided to show the positioning of A-scans $A_{11}, A_{12}, \dots, A_N$ within vessel **101**. Each place where one of A-scans $A_{11}, A_{12}, \dots, A_N$ intersects a surface of a feature within vessel **101** (e.g., a vessel wall) coherent light is reflected and detected. Catheter **826** translates along axis **117** being pushed or pulled by pullback motor **865**.

Looking back at FIG. 6, the reflected, detected light is transmitted along sample path **913** to be recombined with the light from reference path **915** at splitter **919**. Calibration of the system relates to a length of sample path **913** compared to a length of reference path **915**. The difference between these lengths is referred to as the z-offset and when the paths are the same length, the z-offset is said to be zero, and the system is calibrated. Calibration will be discussed in more detail below. Z-offset is discussed in U.S. Pat. No. 8,116,605, the contents of which are hereby incorporated by reference in their entirety for all purposes. When the z-offset is zero, the system is said to be calibrated.

After combining light from the sample, and reference paths, the combined light from splitter **919** is split into orthogonal polarization states, resulting in RF-band polarization-diverse temporal interference fringe signals. The interference fringe signals are converted to photocurrents using PIN photodiodes **929a, 929b, . . .** on the OCB **851** as shown in FIG. 6. The interfering, polarization splitting, and detection steps are done by a polarization diversity module (PDM) on the OCB. Signal from the OCB is sent to the DAQ **855**, shown in FIG. 5. The DAQ includes a digital signal processing (DSP) microprocessor and a field programmable gate array (FPGA) to digitize signals and communicate with the host workstation and the PIM. The FPGA converts raw optical interference signals into meaningful OCT images. The DAQ also compresses data as necessary to reduce image transfer bandwidth to 1 gigabit per second (Gbps) (e.g., compressing frames with a lossy compression JPEG encoder).

Data is collected from A-scans $A_{11}, A_{12}, \dots, A_N$, as shown in FIG. 10, and stored in a tangible, non-transitory memory. A set of A-scans captured in a helical pattern during a rotation and pullback event can be collected and viewed alongside one another in a plane, in a format known as a B-scan.

FIG. 11 gives a reproduction of a B-scan collected using an OCT system. Each horizontal row of pixels corresponds to one A-scan, with the first A-scan (e.g., A_{11}) being displayed across the top of the image. The horizontal axis labeled “Depth” represents a radial distance from imaging catheter **826**. Noting—as shown in FIG. 9—that each A-scan line is progressively displaced from an adjacent A-scan in an angular direction around an axis **117** of catheter **826** (while also being displaced in a translational direction along axis **117**), one set of A-scans associated with a 360° displacement around axis **117** can be collected into a view that depicts a slice of vessel **101** perpendicular to axis **117**. This view is referred to as a tomographic view.

FIG. 12 shows a tomographic view based on the B-scan of FIG. 10. A tomographic view comprises a set of A-scans that defines one circumference around vessel **101**. An arrow pointing straight down in FIG. 11 corresponds to the circular arrow in FIG. 12 and aids in visualization of the three-dimensional nature of the data.

FIG. 13 provides a cartoon illustration of a set of A-scans $A_{11}, A_{12}, \dots, A_{18}$ used to compose a tomographic view. These A-scan lines are shown as would be seen looking down axis **117** (i.e., longitudinal distance between them is not shown). While eight A-scan lines are here illustrated in cartoon format in FIG. 13, typical OCT applications can include between 300 and 1,000 A-scan lines to create a B scan (e.g., about 660) or a tomographic view.

FIG. 14 provides a cartoon illustration of the tomographic view associated with the A-scans of FIG. 13. Reflections detected along each A-scan line are associated with features within the imaged tissue. Reflected light from each A-scan

is combined with corresponding light that was split and sent through reference path **915** and VDL **925** and interference between these two light paths as they are recombined indicates features in the tissue. Where a tomographic view such as is depicted in FIG. **14** generally represents an image as a planar view across a vessel (i.e., normal to axis **117**), an image can also be represented as a planar view along a vessel (i.e., axis **117** lies in the plane of the view).

FIG. **15** shows a longitudinal plane **127** through a vessel **101** including several A scans. Such a planar image along a vessel is sometimes referred to as an in-line digital view or image longitudinal display (ILD). As shown in FIG. **15**, plane **127** generally comprises data associated with a subset of the A scans. The data of the A scan lines is processed according to systems and methods of the inventions to generate images of the tissue. By processing the data appropriately (e.g., by fast Fourier transformation), a two-dimensional image can be prepared from the three dimensional data set. Systems and methods of the invention provide one or more of a tomographic view, ILD, or both.

FIG. **16** is a perspective view of an idealized plane shown including an exemplary ILD in the same perspective as the longitudinal plane shown in FIG. **15**. Where an OCT system captures three-dimensional image data, host workstation **433** may store the three dimensional image data in a tangible, non-transitory memory and provides a display that includes a tomographic view (e.g., FIG. **14**), an ILD (e.g., FIG. **16**), or both (e.g., on a screen or computer monitor). In some embodiments, a tomographic view and an ILD are displayed together, providing information that operators can intuitively visualize as representing a three-dimensional structure.

FIG. **17** is a reproduction of a display of an OCT system including a tomographic view on the left and an ILD on the right. As shown in FIG. **17**, a tomographic view may include ring-like elements near the center and the ILD may include corresponding sets of vertical line-like elements. One ring in the tomographic view may correspond to one pair of lines in the ILD. These elements within the displays are often, in-fact, images of part of the imaging system itself. In some embodiments, a ring in a tomographic view and lines in an ILD represent a surface of catheter **826** such as, for example, an outer surface of a catheter sheath. The portions of the images extending away from those elements are the images of the patient's tissue.

In some embodiments, an OCT system is operated with interchangeable, replaceable, or single-use catheters. Each catheter **826** may provide a different length to sample path **913**. For example, catheters may be used that are designed to be of different lengths, like-manufactured catheters may be subject to imperfect manufacturing tolerances, or catheters may stretch during use. However, to provide a calibrated or scaled image, the z-offset must be known (for post-imaging processing) or set to zero. A z-offset can be known directly (e.g., numerically) or can be known by reviewing an image and determining an apparent difference in an actual location of an element within the image and an expected location of the element within the image.

In some embodiments, the z-offset is calibrated by inspecting an image being captured while they system is running in live mode, and adjusting the actual length of reference path **915** to match the length of sample path **913**.

VDL **925** on reference path **915** uses an adjustable fiber coil to match the length of reference path **915** to the length of sample path **913**. The length of reference path **915** is adjusted by a stepper motor translating a mirror on a translation stage under the control of firmware or software.

The free-space optical beam on the inside of the VDL **925** experiences more delay as the mirror moves away from the fixed input/output fiber. As VDL **925** is adjusted, a length of reference path **915** is known (based, for example, on manufactured specifications of the system).

In some embodiments, the known length of reference path **915** is used to display a calibration mark on a display. If the calibration mark is displayed at a position corresponding to a distal point on reference path **915**, and if sample path **913** is the same length as reference path **915** (e.g., when z-offset is zero), it may be expected that a ring in a tomographic view that represents an outer surface of a catheter sheath will lie along the calibration mark.

When a display includes a calibration mark and a ring-like element representing an outer surface of the catheter sheath separated from one another, an operator has a visual indication that the display is not calibrated.

FIG. **18** is a cartoon illustration of a display **237** including an image of the vessel shown in FIGS. **7A** and **7B**, as rendered by a system of the invention. The images included in display **237** in FIG. **18** are rendered in a simplified style of the purposes of ease of understanding. A system of the invention may render a display as shown in FIG. **17**, or in any style known in the art (e.g., with or without color).

As shown in FIG. **18**, a tomographic view of vessel **101** is depicted alongside an ILD. An outer surface of a catheter sheath appears as a ring **211** in the tomographic view and as lines **217** in the ILD. The tomographic view is depicted as including calibration mark **215**, while calibration mark **219** appears in the ILD.

In some embodiments, z-offset calibration involves precisely determining the position of ring **211** (or lines **217**) in display **237** so that the system can calculate a z-offset based on a known position of calibration mark **215**. Systems of the invention can determine the position of ring **211** or any other calibration element based on user input and an image processing operation. Any suitable user input can be used. In some embodiments discussed below, user input is a "click and drag" operation to move ring **211** to a calibration mark. In certain embodiments, user input is accepted in the form of a single click, a single touch of a touch screen, or some other simple gesture.

FIG. **19** illustrates, in simplified fashion, a display of an imaging system showing a catheter sheath **211** and calibration mark **215**. A user can click on the display near the sheath **211**. In some embodiments, the system detects the location of the catheter sheath with no more input from a user than an indication of a single point. A single point can be input by a mouse-click, a touch on a touchscreen, a light pen or light gun, by "driving" a point to a certain position with arrow keys or a joystick, or by any other suitable method known in the art.

The system can additionally use a processor to perform an image processing operation to detect sheath **211**. In some embodiments, user input indicates a single point **221** on the screen. The system then defines an area around point **221**.

FIG. **20** depicts a defined area **227** around point **221** on a B-scan. Area **227** operates as a search window. The search window area **227** may be a rectangle, circle, ellipse, polygon, or other shape. It may have a predetermined area (e.g., a certain number of pixels). In some embodiments, a size and shape of area **227** is determined by a combination of input device resolution, screen area subtended by a pixel at the particular polar coordinates, current zoom factor, usability studies, or a combination thereof. Usability studies can be performed to establish a statistical model of user repeatability and reproducibility under controlled conditions.

The system searches for the sheath within area **227** by performing a processing operation on the corresponding data. The processing operation can be any suitable search algorithm known in the art.

In some embodiments, a morphological image processing operation is used. Morphological image processing includes operations such as erosion, dilation, opening, and closing, as well as combination thereof. In some embodiments, these operations involve converting the image data to binary data giving each pixel a binary value. With pixels within area **227** converted to binary, each pixel of catheter sheath **211** will be black, and the background pixels will predominantly be white. In erosion, every pixel that is touching background is changed into a background pixel. In dilation, every background pixel that is adjacent to the non-background object pixels is changed into an object pixel. Opening is an erosion followed by a dilation, and closing is a dilation followed by an erosion. Morphological image processing is discussed in Smith, *The Scientist and Engineer's Guide to Digital Signal Processing*, 1997, California Technical Publishing, San Diego, CA, pp. 436-442.

If sheath **211** is not found within area **227**, area **227** can be increased and the increased area can be searched. This strategy can exploit the statistical properties of signal-to-noise ratio (SNR) by which the ability to detect an object is proportional to the square root of its area. See Smith, *Ibid.*, pp. 432-436.

With continued reference to FIG. **20**, once a portion of catheter sheath **211** is detected within area **227**, the search can then be extended "upwards" and "downwards" into adjacent A-scan lines in the B-scan until the entire catheter sheath **211** is detected by the processor and its location is determined with precision. In some embodiments, image processing operations incorporate algorithms with pre-set or user-set parameters that optimize results and continuity of results. For example, if a line appears that is not contiguous across an entire 100% of the image (e.g., the entire extent of the B-scan or a full circle in a tomographic view), an accept or reject parameter can be established based on a percent contiguous factor. In some embodiments, lines that are contiguous across less than 75% (or 50% or 90%, depending on applications) are rejected while others are accepted.

While described above as detecting a reference item (e.g., catheter sheath **211**) by receiving user input followed by using a processor to detect a location of the sheath, the steps can be performed in other orders. For example, the system can apply morphological processing operations to an entire image and detect every element, or every element that satisfies a certain quality criterion. Then the system can receive user input that indicates a point within an image and the user can then choose the pre-detected element that is closest to that point within the image. Similarly, the steps can be performed simultaneously.

Using the methodologies herein, systems of the invention can detect an element within an image of an imaging system, such as an OCT system, with great precision, based on human input that need not be precise and computer processing that need not on its own be accurate. Based on this detection, an actual location of a catheter sheath is determined and thus a precise z-coordinate Z_s for the catheter sheath (e.g., within a B-scan) is known. Where an expected z-coordinate Z_c for the catheter sheath is known, based on information provided extrinsically, the z-offset, and thus a calibration value, can be determined. For example, in FIG. **20**, Z_s is depicted as lying to the right of Z_c , thereby showing a non-zero z-offset. The calibration value is then used to provide a calibrated image, or an image at a known scale.

In some embodiments, the system calculates or uses the mean, median, or root-mean-squared distance of the sheath from the calibration mark to compute the calibration value. This may be advantageous in the event of interfering speckle noise, rough or acylindrical sheaths, non-uniform catheter rotation (NURD), angular displacement of a transducer within the sheath, off-center positioning of the transducer within the sheath, or a combination thereof. In certain embodiments, only a subset of the detected points are used, for example, for efficiency or performance optimization.

FIG. **21** shows a calibrated image, here, a B-scan. The image is depicted having the catheter sheath aligned with the calibration mark. Bars on the left and right side of FIG. **21** show that some data may be shifted out and some blank space introduced by the calibration. In an alternative embodiment, the image can be stretched or compressed, or a combination of stretching and shifting may be performed, depending on preferences, purposes, or functions of a system.

It will be appreciated that the foregoing description is applicable in live mode or review mode. If the imaging system is operating in live mode, capturing an image of tissue, the calibration can be put into effect either by changing the length of reference path **915** so that z-offset is zero or by transforming the dataset or on-screen image. The length of reference path **915** can be changed through the operation of the motor in the VDL. The distance $Z_c - Z_s$ is converted into millimeters and the a command is sent to move the VDL to a new position.

If the dataset is to be transformed, either in live mode or while the system is operating in review mode, the system is digitally shifted, stretched, or a combination thereof.

In another aspect, the invention provides a method for calibrating an imaging system based on receipt of user input that indicates a "motion", such as a click-and-drag operation on a computer screen.

FIGS. **22** and **23** illustrate receiving user input indicating a motion through a mouse dragging operation. User input could also be a drag on a touchscreen or other input (arrow keys, pointer, trackball, etc.) As depicted in FIGS. **22-23**, a user clicks on a reference item (e.g., sheath **211**) with a mouse and drags it to a new position, for example, onto a calibration mark or other position on the display. The system (e.g., using a processor) can then calculate a calibration value based on indicated motion of the reference item.

This method allows a user to manually calibrate or apply any offset using a drag-and-drop operation on the tomographic view or on the ILD. While dragging, the distance between the grab point and current point represented by the tip of the mouse pointer (or analogous finger-touch point in touchscreens) may be continuously calculated. In live mode, the image may be shifted digitally or by moving the VDL and in review mode the image is transformed digitally, as discussed above.

FIG. **24** shows releasing a click-and-drag motion. In some embodiments, the image is shifted (digitally or by moving the VDL) simultaneously with the user's drag motion. In certain embodiments, the system begins the shift after the user completes the drag input motion. (Note that in FIGS. **23** and **24** a dotted line is shown to represent the original location of the catheter sheath, and the dotted line is not meant to represent a calibration mark. A calibration mark is optional.)

While discussed above using a surface of a catheter sheath as a reference item which is used as a basis for calibration, other reference items are suitable. For example, any item that can be depicted such that its expected location and

actual location can be compared in a display of an imaging system may be used. In some embodiments, a fiducial marker or calibration bar is introduced into the imaging target having a known dimension (e.g., 1 nm, 1 mm, 1 cm). The system operates to display a scale or a grid based on an expected appearance of the known dimension. The user then gives input indicating a point in the display near the reference item and the system also detects a location of the reference item in an area around the indicated point. Based on the expected and actual locations or dimensions of the reference item, a calibration value is calculated and a calibrated image is provided. User input, displays, and methods of receiving user input and performing calculations may be provided by one or more computers.

In certain embodiments, display 237 is rendered within a computer operating system environment, such as Windows, Mac OS, or Linux or within a display or GUI of a specialized system. Display 237 can include any standard controls associated with a display (e.g., within a windowing environment) including minimize and close buttons, scroll bars, menus, and window resizing controls. Elements of display 237 can be provided by an operating system, windows environment, application programming interface (API), web browser, program, or combination thereof (for example, in some embodiments a computer includes an operating system in which an independent program such as a web browser runs and the independent program supplies one or more of an API to render elements of a GUI). Display 237 can further include any controls or information related to viewing images (e.g., zoom, color controls, brightness/contrast) or handling files comprising three-dimensional image data (e.g., open, save, close, select, cut, delete, etc.). Further, display 237 can include controls (e.g., buttons, sliders, tabs, switches) related to operating a three dimensional image capture system (e.g., go, stop, pause, power up, power down).

In certain embodiments, display 237 includes controls related to three dimensional imaging systems that are operable with different imaging modalities. For example, display 237 may include start, stop, zoom, save, etc., buttons, and be rendered by a computer program that interoperates with OCT or IVUS modalities. Thus display 237 can display an image derived from a three-dimensional data set with or without regard to the imaging mode of the system.

FIG. 25 diagrams an exemplary system 400. As shown in FIG. 25, imaging engine 859 communicates with host workstation 433 as well as optionally server 413 over network 409. In some embodiments, an operator uses host workstation 433, computer 449, or terminal 467 to control system 400 or to receive images. An image may be displayed using an I/O 454, 437, or 471, which may include a monitor. Any I/O may include a monitor, keyboard, mouse or touchscreen to communicate with any of processor 421, 459, 441, or 475, for example, to cause data to be stored in any tangible, nontransitory memory 463, 445, 479, or 429. Server 413 generally includes an interface module 425 to communicate over network 409 or write data to data file 417. Input from a user is received by a processor in an electronic device such as, for example, host workstation 433, server 413, or computer 449. Methods of the invention can be performed using software, hardware, firmware, hardwiring, or combinations of any of these. Features implementing functions can also be physically located at various positions, including being distributed such that portions of functions are implemented at different physical locations (e.g., imaging apparatus in one room and host workstation in another, or in separate buildings, for example, with wireless or wired connections). In

certain embodiments, host workstation 433 and imaging engine 855 are included in a bedside console unit to operate system 400.

A computer generally includes a processor for executing instructions and one or more memory devices for storing instructions, data, or both. Processors suitable for the execution of methods and operations described herein include, by way of example, both general and special purpose microprocessors (e.g., an Intel chip, an AMD chip, an FPGA). Generally, a processor will receive instructions or data from read-only memory, random access memory, or both. Generally, a computer will also include, or be operatively coupled, one or more mass storage devices for storing data that represent target such as bodily tissue. Any suitable computer-readable storage device may be used such as, for example, solid-state, magnetic, magneto-optical disks, or optical disks. Information carriers suitable for embodying computer program instructions and data include all forms of non-volatile memory, particularly tangible, non-transitory memory including by way of example semiconductor memory devices, (e.g., EPROM, EEPROM, NAND-based flash memory, solid state drive (SSD), and other flash memory devices); magnetic disks, (e.g., internal hard disks or removable disks); magneto-optical disks; and optical disks (e.g., CD and DVD disks).

INCORPORATION BY REFERENCE

References and citations to other documents, such as patents, patent applications, patent publications, journals, books, papers, web contents, have been made throughout this disclosure. All such documents are hereby incorporated herein by reference in their entirety for all purposes.

EQUIVALENTS

Various modifications of the invention and many further embodiments thereof, in addition to those shown and described herein, will become apparent to those skilled in the art from the full contents of this document, including references to the scientific and patent literature cited herein. The subject matter herein contains important information, exemplification and guidance that can be adapted to the practice of this invention in its various embodiments and equivalents thereof.

The invention claimed is:

1. An imaging system, comprising:
 - an intravascular imaging catheter configured to be positioned within a vessel of a patient; and
 - a processor configured for communication with the intravascular imaging catheter, wherein the processor is configured to:
 - receive, from the intravascular imaging catheter, a first intravascular image including the vessel and a reference item;
 - output, to a display in communication with the processor, the first intravascular image including the vessel and the reference item;
 - receive a user input to move the displayed reference item from a first position to a second position, wherein the first position comprises a first diameter, wherein the second position comprises a second diameter different from the first diameter;
 - determine a calibration value based on a difference between the first diameter and the second diameter;
 - generate, in response to determining the calibration value based on the difference between the first diam-

15

- eter and the second diameter, a second intravascular image of the vessel, wherein the second intravascular image is a transformation of the first intravascular image based on the calibration value; and
output, to the display without conducting a new scan, the second intravascular image of the vessel.
2. The system of claim 1, wherein the reference item comprises a structure of the intravascular imaging catheter disposed within the vessel.
3. The system of claim 2, wherein the reference item comprises a catheter sheath.
4. The system of claim 1, wherein the calibration value comprises a z-offset associated with an interferometric device.
5. The system of claim 1, wherein the user input comprises a start and an end, and wherein the processor is configured to determine the calibration value in response to the start of the user input.
6. The system of claim 1, wherein the user input comprises a start and an end, and wherein the processor is configured to determine the calibration value in response to the end of the user input.
7. The system of claim 1, wherein the user input comprises a click-and-drag motion.
8. The system of claim 1, wherein, to generate the second intravascular image of the vessel, the processor is configured to:
digitally transform the first intravascular image based on the user input.
9. The system of claim 8, wherein, to digitally transform the first intravascular image, the processor is configured to at least one of stretch, shift, or compress the first intravascular image.
10. The system of claim 1, wherein the imaging system is an optical coherence tomography system comprising a reference path and a sample path, and wherein, to generate the second intravascular image of the vessel, the processor is configured to:
adjust a length of the reference path based on the calibration value; and
receive the second intravascular image of the vessel from the intravascular imaging catheter via the sample path, wherein the second intravascular image of the vessel is obtained with respect to the adjusted length of the reference path.
11. The system of claim 10, wherein the reference path comprises a variable delay line, and wherein, to adjust the length of the reference path, the processor is configured to operate a motor of the variable delay line.
12. The system of claim 2, wherein the first diameter comprises a diameter of the structure of the intravascular imaging catheter in the first intravascular image, wherein the second diameter comprises a diameter of the structure of the intravascular imaging catheter in the second intravascular image, and wherein the user input to move the displayed reference item from the first position to the second position

16

- comprises a change to the displayed reference item from the first diameter to the second diameter.
13. A method, comprising:
receiving, from an intravascular imaging catheter positioned within a vessel of a patient, a first intravascular image including the vessel and a reference item;
outputting, to a display, the first intravascular image including the vessel and the reference item;
receiving a user input to move the displayed reference item from a first position to a second position, wherein the first position comprises a first diameter, wherein the second position comprises a second diameter different from the first diameter;
determining a calibration value based on a difference between the first diameter and the second diameter;
generating, in response to determining the calibration value based on the difference between the first diameter and the second diameter, a second intravascular image of the vessel, wherein the second intravascular image is a transformation of the first intravascular image based on the calibration value; and
outputting, to the display without conducting a new scan, the second intravascular image of the vessel.
14. The method of claim 13, wherein the reference item comprises a structure of the intravascular imaging catheter disposed within the vessel.
15. The method of claim 14, wherein the reference item comprises a catheter sheath.
16. The method of claim 13, wherein the calibration value comprises a z-offset associated with an interferometric device.
17. The method of claim 13, wherein receiving the user input comprises a start and an end, and wherein determining the calibration value is in response to the start of the user input.
18. The method of claim 13, wherein receiving the user input comprises a start and an end, and wherein determining the calibration value is in response to the end of the user input.
19. The method of claim 13, wherein the user input comprises a click-and-drag motion.
20. The method of claim 13, wherein generating the second intravascular image of the vessel comprises digitally transforming the first intravascular image based on the user input.
21. The method of claim 13, wherein generating the second intravascular image of the vessel comprises:
adjusting a length of a reference path based on the calibration value; and
receiving the second intravascular image of the vessel from the intravascular imaging catheter via a sample path, wherein the second intravascular image of the vessel is obtained with respect to the adjusted length of the reference path, wherein the reference path comprises a variable delay line, and wherein adjusting the length of the reference path comprises operating a motor of the variable delay line.