



US012072288B2

(12) **United States Patent**  
**Han et al.**

(10) **Patent No.:** **US 12,072,288 B2**  
(45) **Date of Patent:** **Aug. 27, 2024**

(54) **MULTIPLE LIGHT PATHS ARCHITECTURE AND OBSCURATION METHODS FOR SIGNAL AND PERFUSION INDEX OPTIMIZATION**

(58) **Field of Classification Search**  
CPC ..... A61B 5/0059; A61B 5/681; A61B 5/6802; A61B 5/6898; A61B 5/02416;  
(Continued)

(71) Applicant: **Apple Inc.**, Cupertino, CA (US)

(56) **References Cited**

(72) Inventors: **Chin San Han**, Mountain View, CA (US); **Ueyn Block**, Menlo Park, CA (US); **Brian R. Land**, Woodside, CA (US); **Nevzat Akin Kestelli**, San Jose, CA (US); **Serhan Isikman**, Sunnyvale, CA (US); **Albert Wang**, Sunnyvale, CA (US); **Justin Shi**, Santa Clara, CA (US)

U.S. PATENT DOCUMENTS

5,246,002 A 9/1993 Prosser  
5,273,036 A 12/1993 Kronberg et al.  
(Continued)

(73) Assignee: **Apple Inc.**, Cupertino, CA (US)

FOREIGN PATENT DOCUMENTS

CN 100381095 4/2008  
CN 101108126 6/2010  
(Continued)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

OTHER PUBLICATIONS

Shi, V. et al. (Jul. 20, 2009). "Non-contact Reflection Photoplethysmography Towards Effective Human Physiological Monitoring," *Journal of Medical and Biomedical Engineering*, 30(3), 161-167.

(21) Appl. No.: **18/084,342**

*Primary Examiner* — Amelie R Davis

(22) Filed: **Dec. 19, 2022**

(74) *Attorney, Agent, or Firm* — Brownstein Hyatt Farber & Schreck, LLP

(65) **Prior Publication Data**

US 2023/0204506 A1 Jun. 29, 2023

**Related U.S. Application Data**

(63) Continuation of application No. 16/144,958, filed on Sep. 27, 2018, now Pat. No. 11,536,653, which is a  
(Continued)


(57) **ABSTRACT**

A photoplethysmographic (PPG) device is disclosed. The PPG device can include one or more light emitters and one or more light sensors to generate the multiple light paths for measuring a PPG signal and perfusion indices of a user. The multiple light paths between each pair of light emitters and light detectors can include different separation distances to generate both an accurate PPG signal and a perfusion index value to accommodate a variety of users and usage conditions. In some examples, the multiple light paths can include the same separation distances for noise cancellation due to artifacts resulting from, for example, tilt and/or pull of the device, a user's hair, a user's skin pigmentation, and/or motion. The PPG device can further include one or more lenses and/or reflectors to increase the signal strength and/or  
(Continued)

(51) **Int. Cl.**  
**A61B 5/00** (2006.01)  
**A61B 5/024** (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **G01N 21/4738** (2013.01); **A61B 5/0059** (2013.01); **G01N 21/55** (2013.01);  
(Continued)

Device  
700

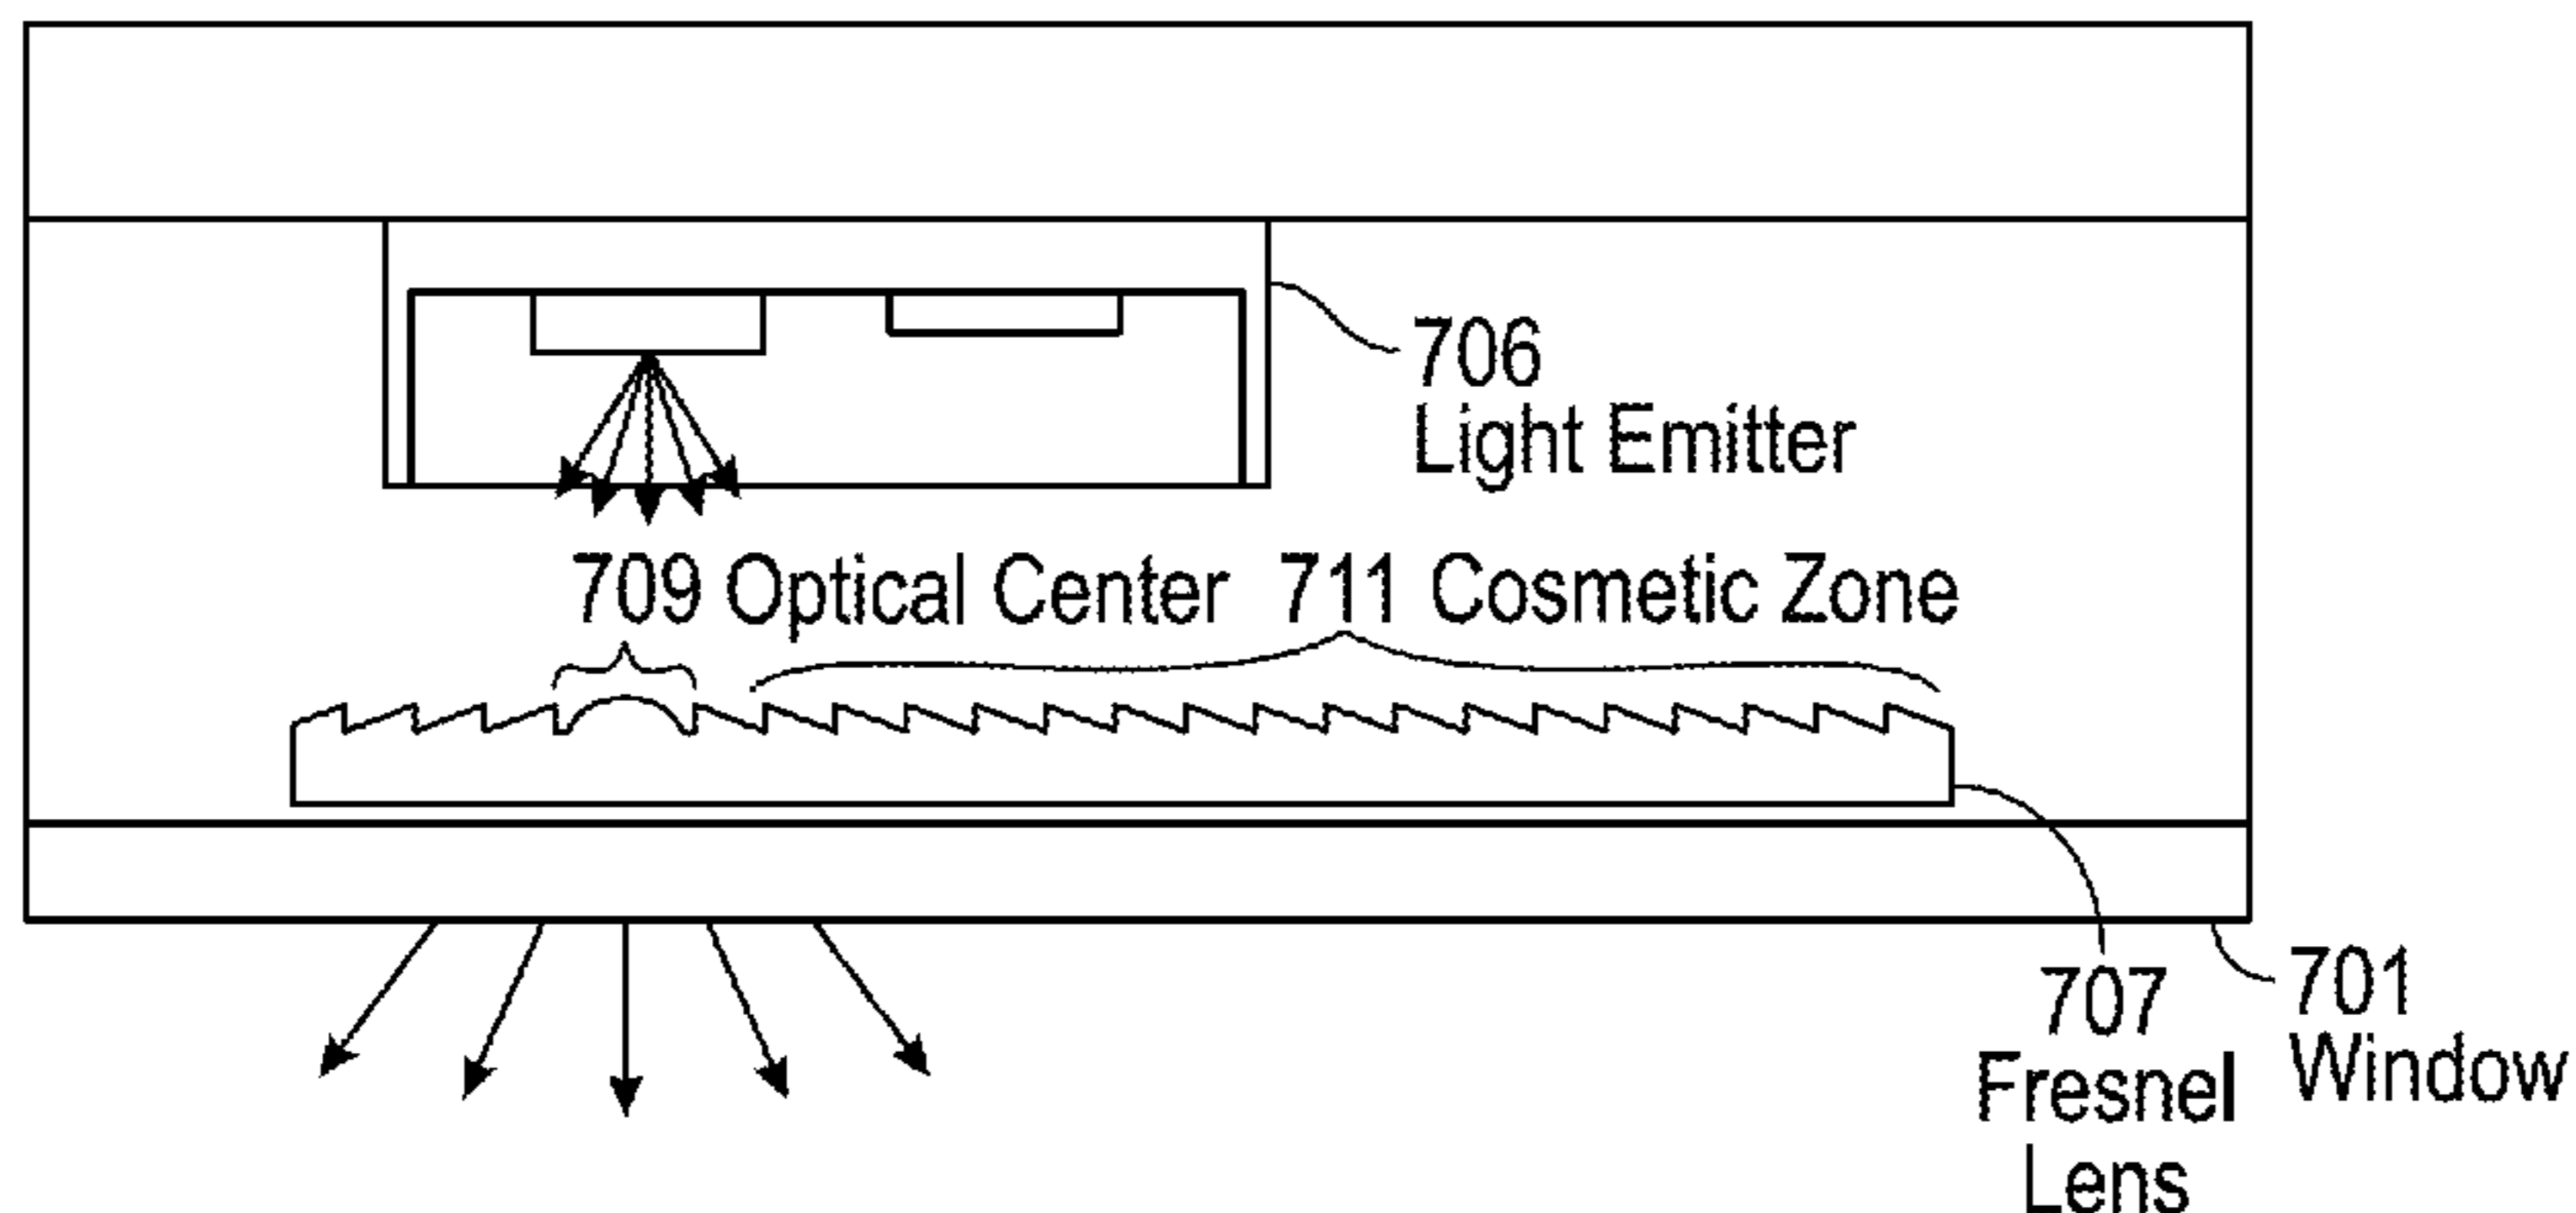

and to obscure the optical components and associated wiring from being visible to a user's eye.

**20 Claims, 13 Drawing Sheets**

**Related U.S. Application Data**

continuation of application No. 14/569,235, filed on Dec. 12, 2014, now Pat. No. 10,215,698.

(60) Provisional application No. 62/044,515, filed on Sep. 2, 2014.

(51) **Int. Cl.**  
**G01N 21/47** (2006.01)  
**G01N 21/55** (2014.01)

(52) **U.S. Cl.**  
 CPC ..... *A61B 5/02416* (2013.01); *A61B 5/681* (2013.01); *A61B 5/6898* (2013.01); *A61B 5/7203* (2013.01); *A61B 2560/0475* (2013.01); *A61B 2562/0233* (2013.01); *G01N 2201/0638* (2013.01); *G01N 2201/068* (2013.01)

(58) **Field of Classification Search**  
 CPC .. *A61B 5/7203*; *G01N 21/4738*; *G01N 21/55*; *G01N 2201/0638*; *G01N 2201/068*  
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,483,261 A 1/1996 Yasutake  
 5,488,204 A 1/1996 Mead  
 5,759,156 A 6/1998 Hayakawa et al.  
 5,782,237 A 7/1998 Casciani  
 5,825,352 A 10/1998 Bisset et al.  
 5,835,079 A 11/1998 Shieh  
 5,880,411 A 3/1999 Gillespie et al.  
 6,031,603 A 2/2000 Fine et al.  
 6,115,621 A 9/2000 Chin  
 6,188,391 B1 2/2001 Seely et al.  
 6,277,067 B1 8/2001 Blair  
 6,310,610 B1 10/2001 Beaton et al.  
 6,343,233 B1 1/2002 Chin et al.  
 6,491,647 B1 12/2002 Bridger  
 6,529,754 B2 3/2003 Kondo  
 6,533,729 B1 3/2003 Khair et al.  
 6,587,703 B2 7/2003 Cheng et al.  
 6,594,513 B1 7/2003 Jobsis et al.  
 6,690,387 B2 2/2004 Zimmerman et al.  
 6,859,658 B1 2/2005 Krug  
 7,015,894 B2 3/2006 Morohoshi  
 7,030,365 B2 4/2006 Langland  
 7,139,076 B1 11/2006 Marbach  
 7,184,064 B2 2/2007 Zimmerman et al.  
 7,204,606 B2 4/2007 Brass et al.  
 7,372,778 B2 5/2008 Klopfenstein et al.  
 7,450,799 B2 11/2008 Selbrede et al.  
 7,616,110 B2 11/2009 Crump et al.  
 7,643,153 B2 1/2010 de Boer et al.  
 7,663,607 B2 2/2010 Hotelling et al.  
 7,676,253 B2 3/2010 Rarldan, Jr.  
 7,729,748 B2 6/2010 Florian  
 7,740,589 B2 6/2010 Maschke et al.  
 7,890,153 B2 2/2011 Hoarau  
 8,005,624 B1 8/2011 Starr  
 8,086,301 B2 12/2011 Cho et al.  
 8,135,447 B2 3/2012 Kondoh et al.  
 8,203,704 B2 6/2012 Merritt et al.  
 8,252,369 B2 8/2012 Jiang  
 8,378,811 B2 2/2013 Crump et al.  
 8,380,272 B2 2/2013 Barrett et al.

8,588,878 B2 11/2013 Li et al.  
 8,618,930 B2 12/2013 Papadopoulos et al.  
 8,704,152 B2 4/2014 Svajda et al.  
 8,788,002 B2 7/2014 Leboeuf et al.  
 8,803,745 B2 8/2014 Dabov  
 8,805,302 B2 8/2014 Pantfoerder  
 8,948,832 B2 2/2015 Hong et al.  
 8,974,396 B1 3/2015 Brady  
 8,998,815 B2 4/2015 Venkatraman et al.  
 9,008,742 B2 4/2015 Naganuma et al.  
 9,044,149 B2 6/2015 Richards et al.  
 9,049,998 B2 6/2015 Brumback et al.  
 9,113,793 B2 8/2015 Terumoto et al.  
 9,310,843 B2 4/2016 Shedletsy et al.  
 9,314,197 B2 4/2016 Eisen et al.  
 9,322,901 B2 4/2016 Kerness et al.  
 9,326,711 B2 5/2016 Kracker et al.  
 9,348,322 B2 5/2016 Fraser et al.  
 9,392,946 B1 7/2016 Sarantos  
 9,449,955 B2 9/2016 Tu et al.  
 9,506,802 B2 11/2016 Chu et al.  
 9,526,421 B2 12/2016 Papadopoulos et al.  
 9,596,990 B2 3/2017 Park et al.  
 9,651,421 B2 5/2017 Svajda et al.  
 9,737,221 B2 8/2017 Sato  
 9,826,905 B2 11/2017 Addison et al.  
 9,907,510 B2 3/2018 Yoshida et al.  
 10,058,254 B2 8/2018 Fei  
 10,060,788 B2 8/2018 Fei  
 10,092,197 B2 10/2018 Han et al.  
 10,117,587 B2 11/2018 Han et al.  
 10,165,951 B2 1/2019 Rimoldi et al.  
 10,172,529 B2 1/2019 Fei  
 10,180,235 B2 1/2019 Rudmann et al.  
 10,206,589 B2 2/2019 Walker  
 10,215,698 B2 2/2019 Han et al.  
 10,219,729 B2 3/2019 Kintz et al.  
 10,247,670 B2 4/2019 Ness et al.  
 10,265,003 B2 4/2019 Eguchi et al.  
 10,265,024 B2 4/2019 Lee et al.  
 10,266,320 B2 4/2019 McKenzie et al.  
 10,299,724 B2 5/2019 Meitav  
 10,646,143 B2 5/2020 Wang  
 10,687,717 B1 6/2020 Peterson  
 10,694,997 B2 6/2020 Kim et al.  
 10,732,574 B2 8/2020 Shim et al.  
 10,799,128 B2 10/2020 Paulussen et al.  
 10,831,755 B2 11/2020 Ikeda et al.  
 10,907,844 B2 2/2021 Ribbich et al.  
 10,918,322 B2 2/2021 Shao et al.  
 11,206,989 B2 12/2021 Nadeau et al.  
 11,266,320 B2 3/2022 Block et al.  
 11,536,653 B2 12/2022 Han et al.  
 11,627,887 B2 4/2023 Peterson et al.  
 2002/0042558 A1 4/2002 Mendelson  
 2002/0188210 A1 12/2002 Aizawa  
 2004/0032728 A1 2/2004 Galli  
 2008/0004510 A1 1/2008 Tanzawa et al.  
 2008/0297788 A1 12/2008 Rowe et al.  
 2009/0018452 A1 1/2009 Sugiura et al.  
 2009/0182208 A1 7/2009 Cho et al.  
 2010/0056934 A1 3/2010 Cho et al.  
 2010/0113948 A1 5/2010 Yang et al.  
 2011/0077537 A1 3/2011 Ebara et al.  
 2011/0260176 A1 10/2011 Onoe et al.  
 2012/0078116 A1 3/2012 Yamashita  
 2012/0223231 A1 9/2012 Nijaguna  
 2013/0006074 A1 1/2013 Pologe  
 2013/0046192 A1 2/2013 Lin et al.  
 2013/0060098 A1 3/2013 Thomsen et al.  
 2013/0289414 A1 10/2013 Adibnazari et al.  
 2013/0324866 A1 12/2013 Gladshstein  
 2014/0024905 A1 1/2014 Sarrafzadeh et al.  
 2014/0187992 A1 7/2014 Wilmering  
 2015/0065830 A1 3/2015 Karp et al.  
 2015/0234188 A1 8/2015 Lee  
 2016/0113530 A1 4/2016 Nagahiro et al.  
 2016/0198962 A1 7/2016 Park et al.  
 2016/0235369 A1 8/2016 Horikawa et al.

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2016/0242659 A1 8/2016 Yamashita et al.  
 2017/0347902 A1 12/2017 Van Gool et al.  
 2018/0049702 A1 2/2018 Tsai  
 2018/0054077 A1 2/2018 Brzezinski et al.  
 2019/0000331 A1 1/2019 Han  
 2019/0018173 A1 1/2019 Kim et al.  
 2019/0069781 A1 3/2019 Kim et al.  
 2021/0161444 A1 6/2021 Shao et al.  
 2022/0167864 A1 6/2022 Block et al.  
 2023/0248251 A1 8/2023 Peterson et al.

FOREIGN PATENT DOCUMENTS

CN 101730503 6/2010  
 CN 103327894 9/2013  
 CN 103610467 3/2014  
 CN 205054183 3/2016  
 EP 1946697 7/2008  
 EP 2992821 3/2016  
 EP 3117762 1/2017  
 EP 3111834 4/2017  
 GB 2524160 9/2015  
 GB 2547736 8/2017  
 JP 57093039 6/1982  
 JP H02031734 2/1990

JP H11128184 5/1999  
 JP 2000163031 6/2000  
 JP 2002342033 11/2002  
 JP 2002345760 12/2002  
 JP 2005040608 2/2005  
 JP 2008264302 11/2008  
 JP 2011251007 12/2011  
 JP 2013094482 5/2013  
 JP 2013118922 6/2013  
 JP 2016158701 9/2016  
 KR 0100091592 8/2010  
 KR 20140145392 12/2014  
 TW 201806548 3/2018  
 WO WO 19/067196 8/1995  
 WO WO 95/020757 8/1995  
 WO WO 01/117420 3/2001  
 WO WO 07/122375 11/2007  
 WO WO 09/139029 11/2009  
 WO WO 12/011029 1/2012  
 WO WO 12/158384 11/2012  
 WO WO 12/158386 11/2012  
 WO WO 12/158387 11/2012  
 WO WO 14/043410 3/2014  
 WO WO 14/066791 5/2014  
 WO WO 15/084375 6/2015  
 WO WO 15/094378 6/2015  
 WO WO 15/122980 8/2015  
 WO WO 16/032682 3/2016

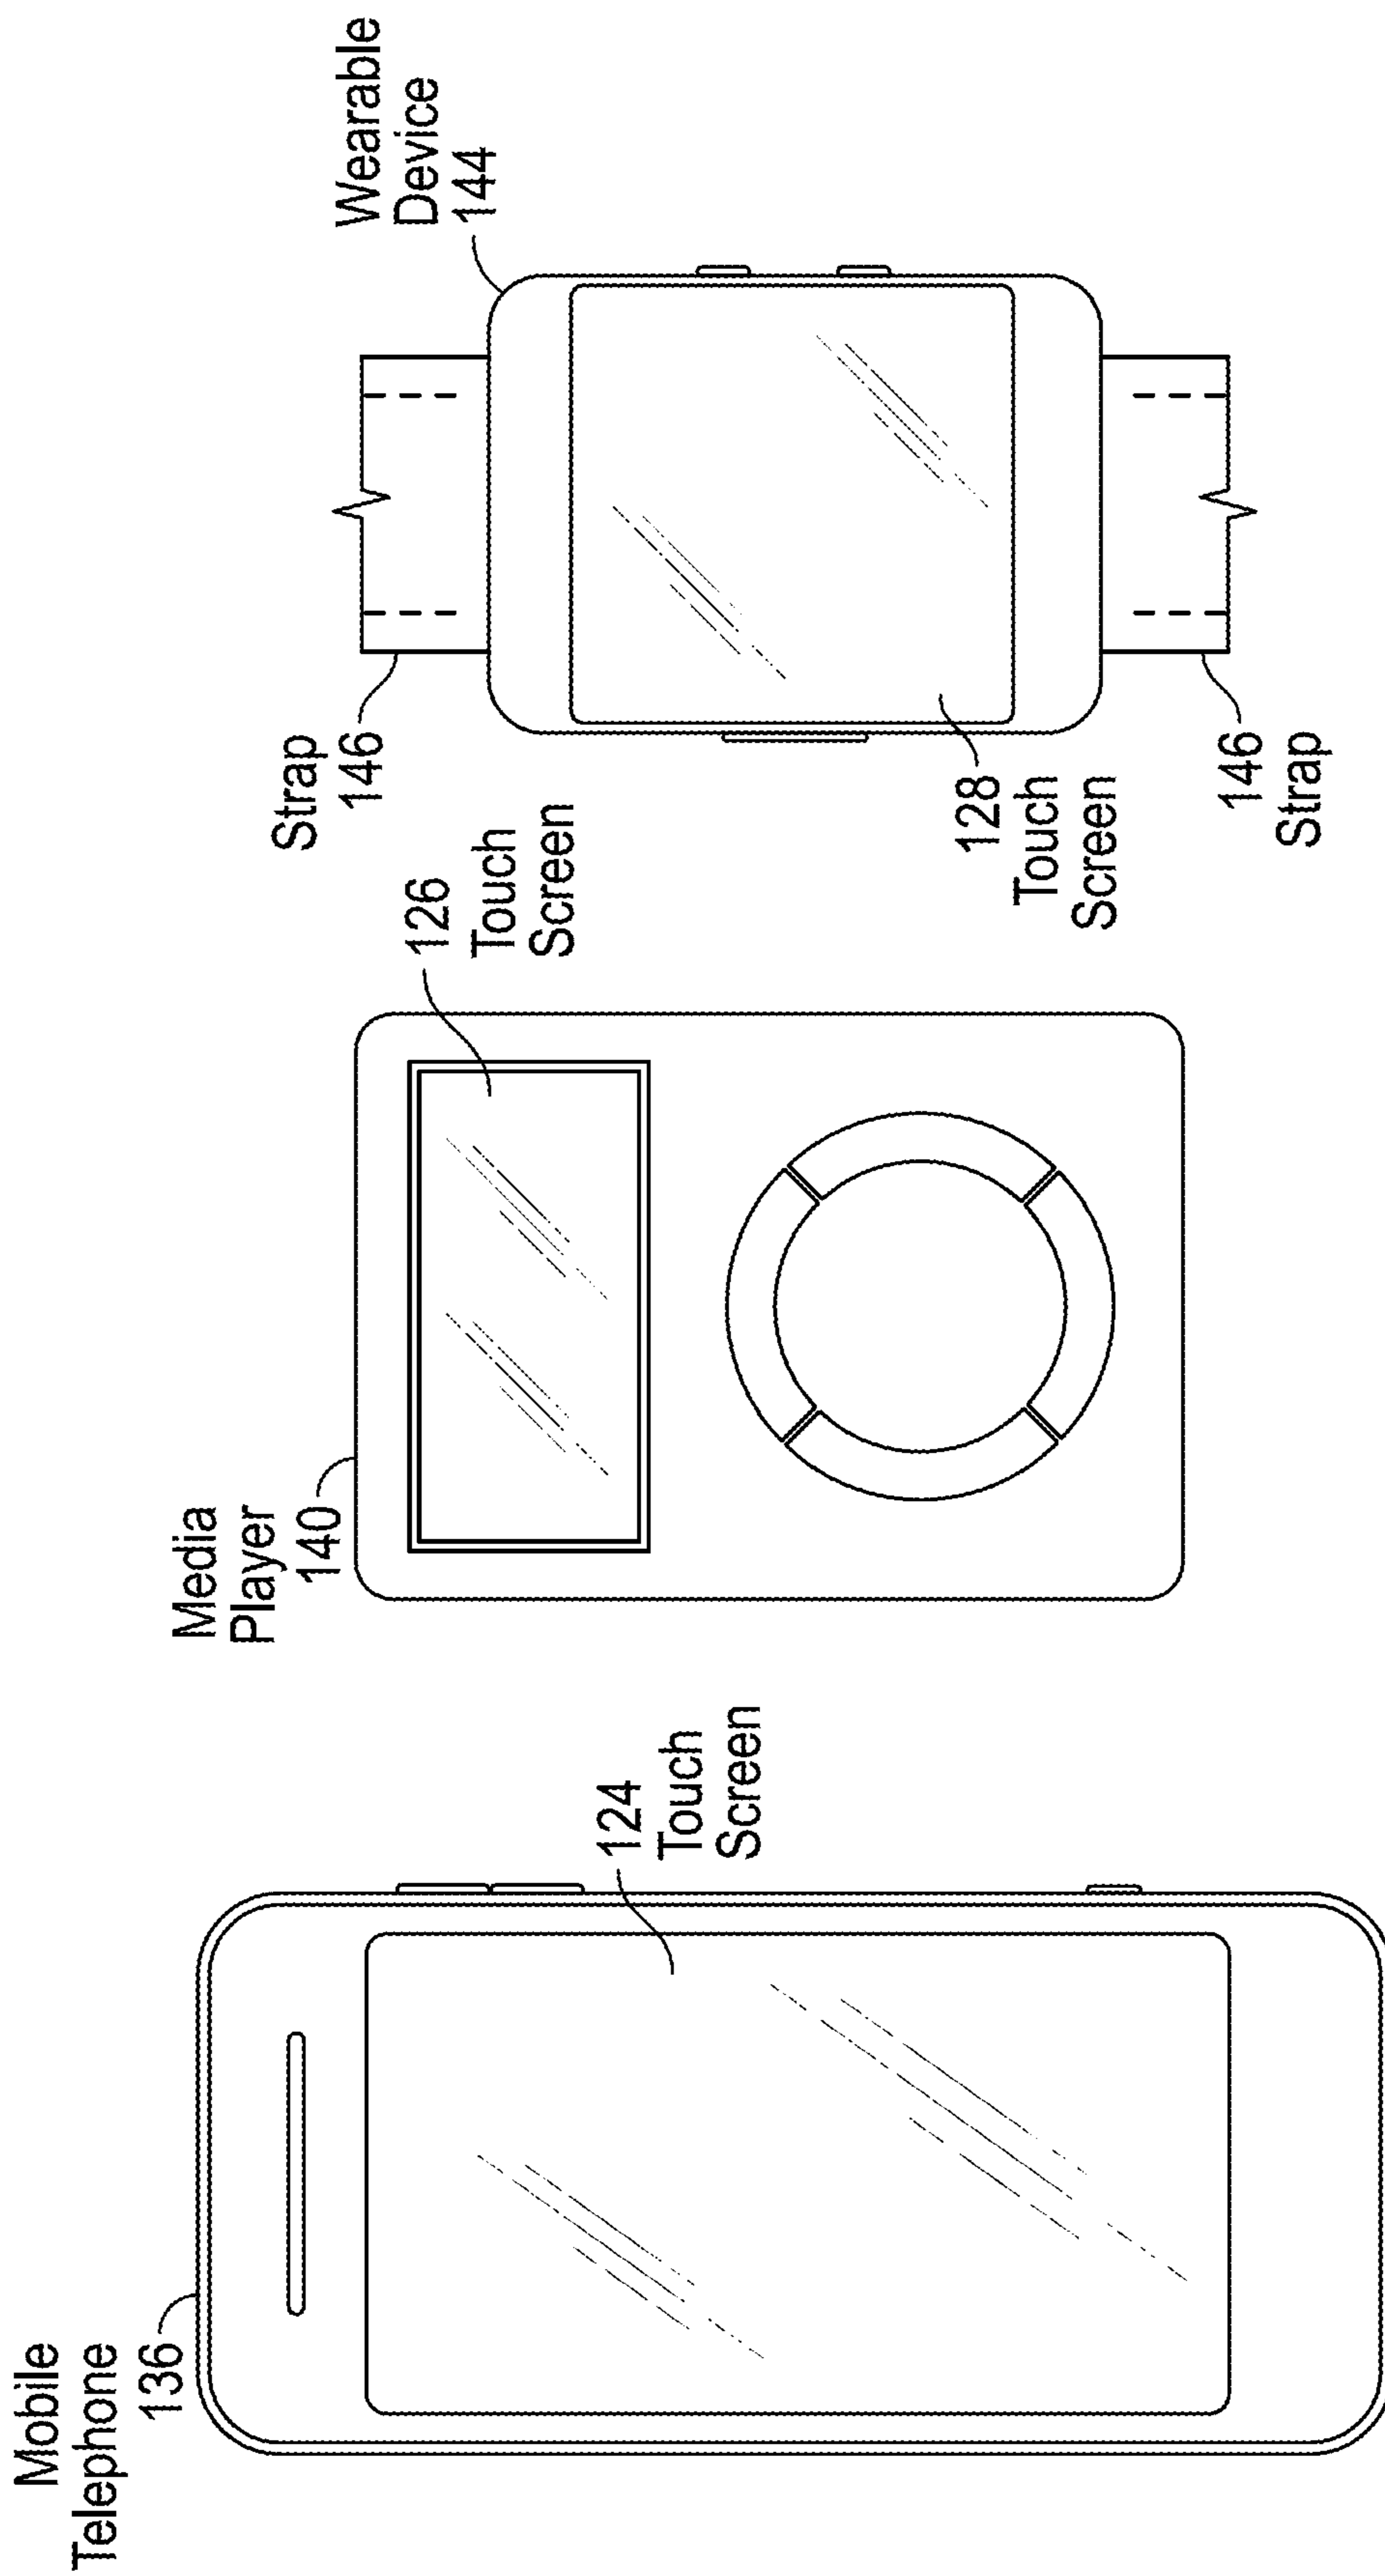


FIG. 1A

FIG. 1B

FIG. 1C

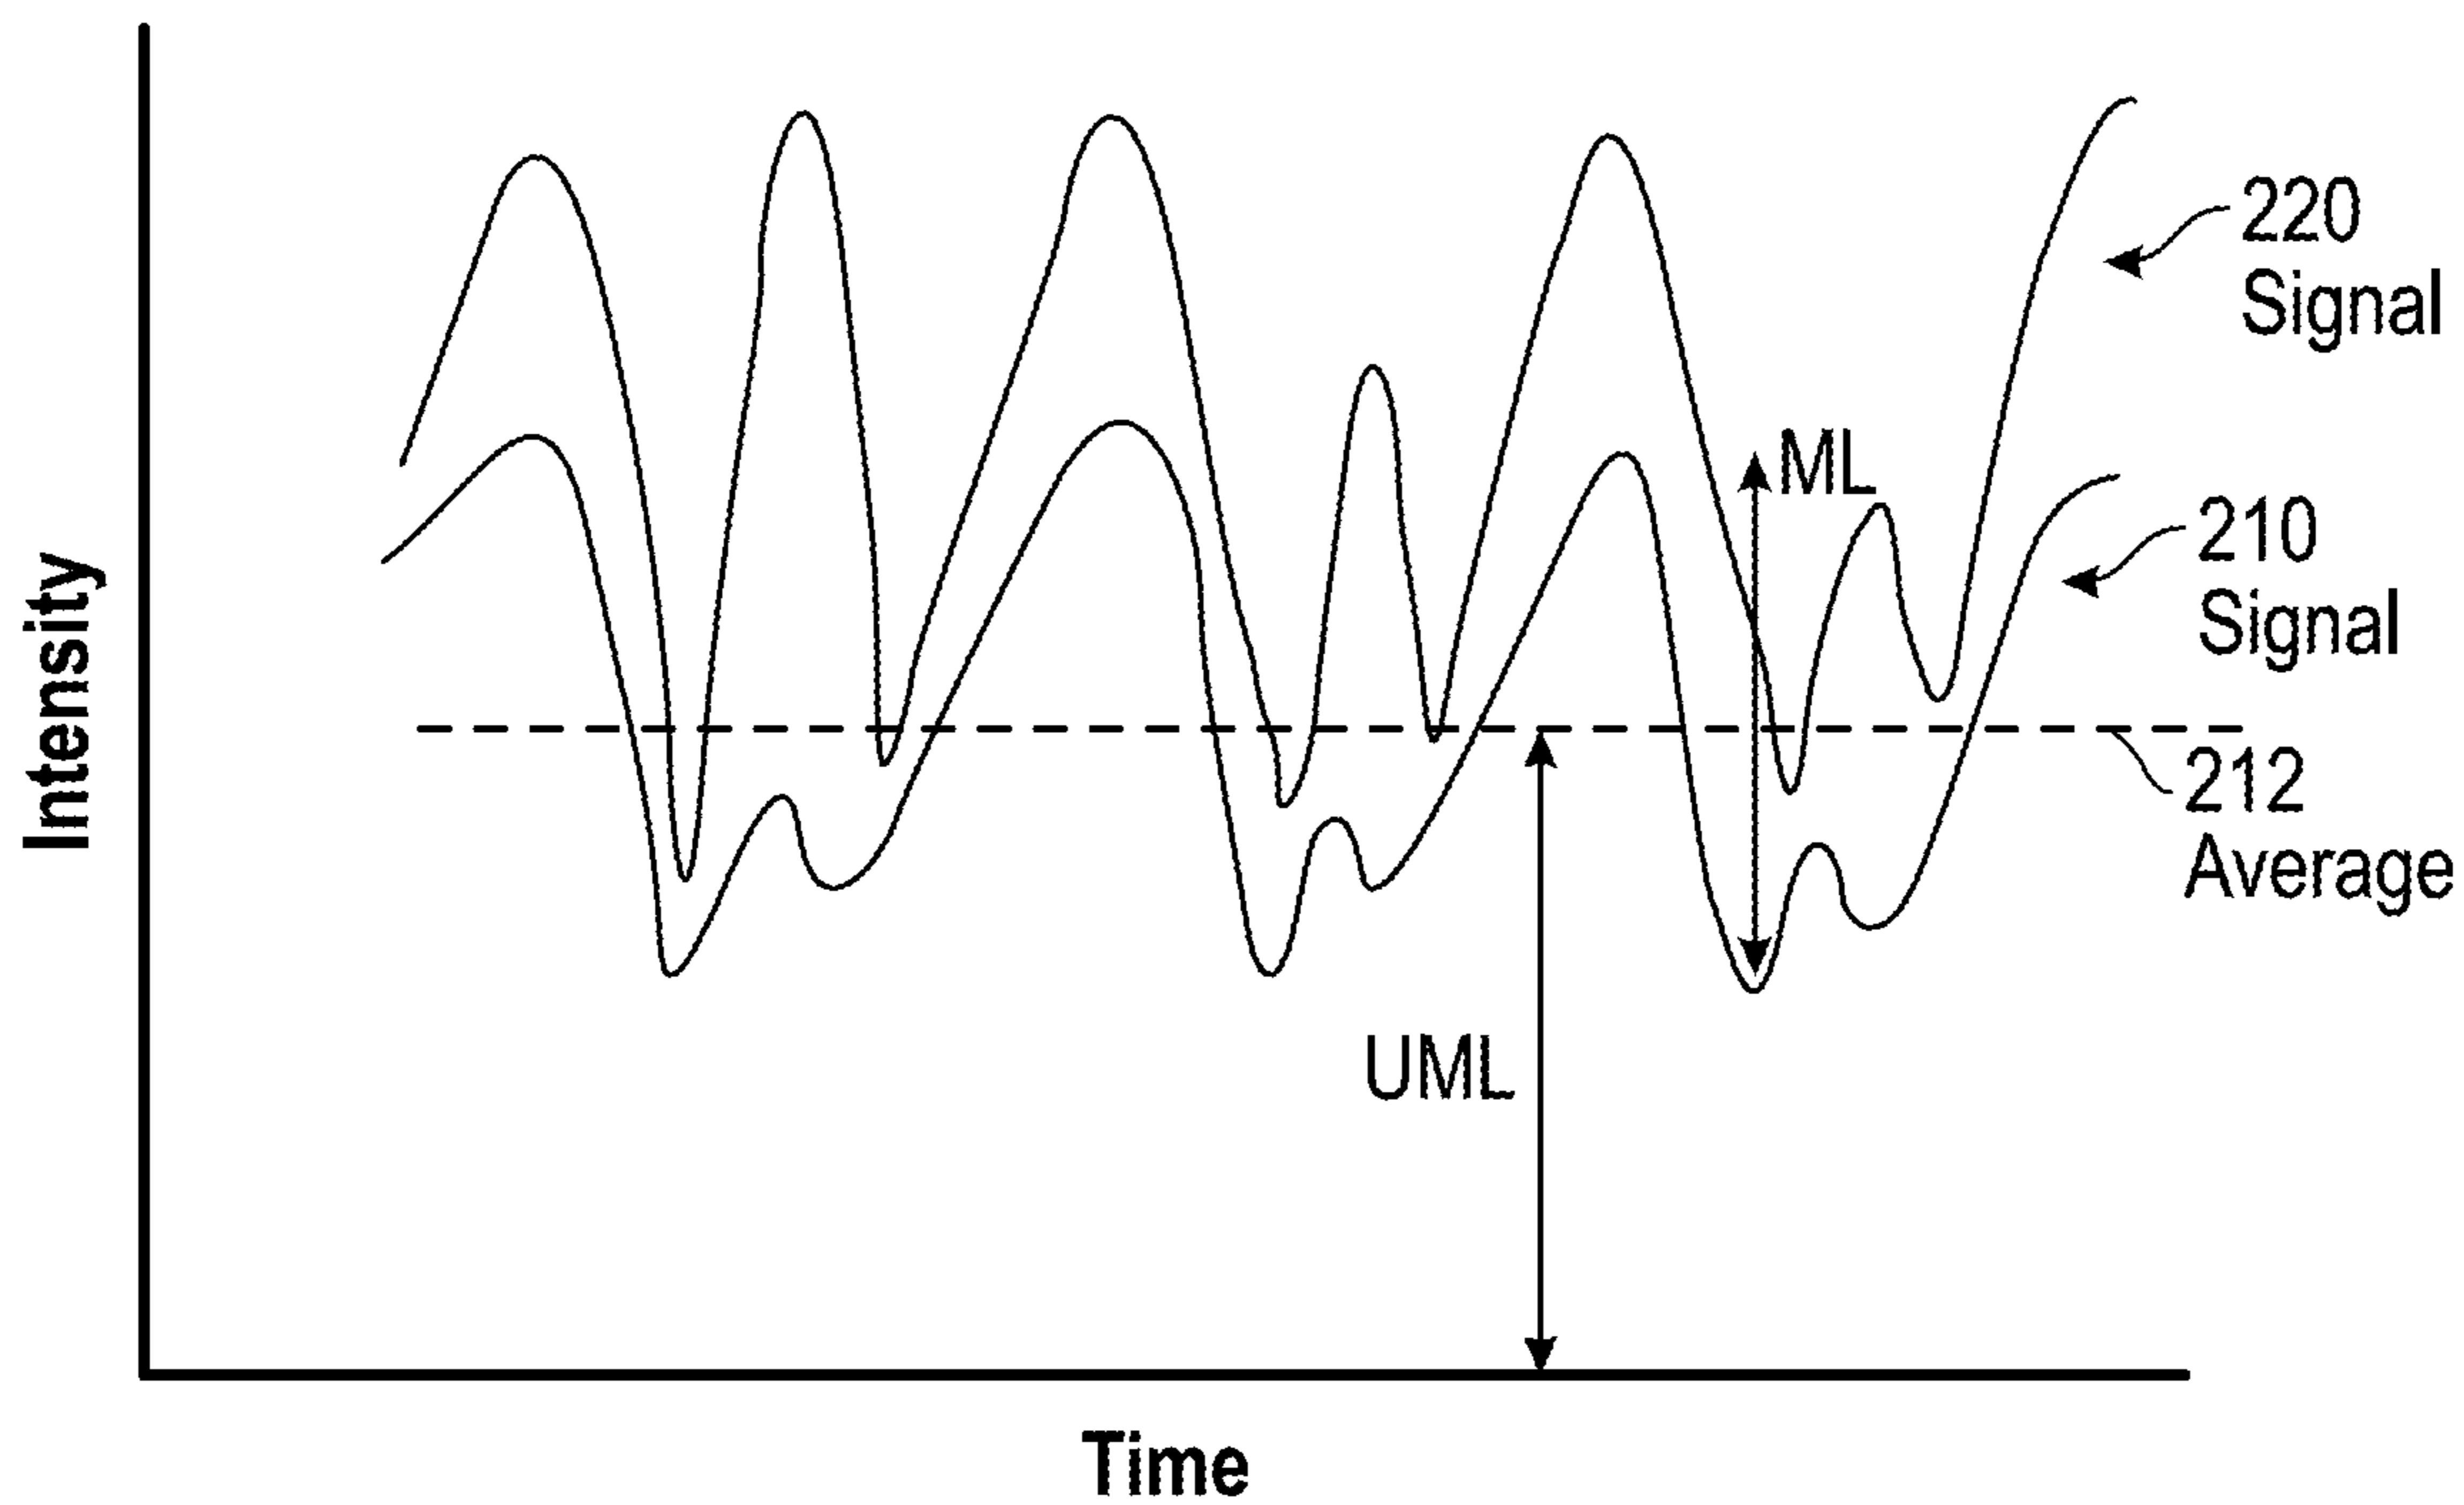


FIG. 2

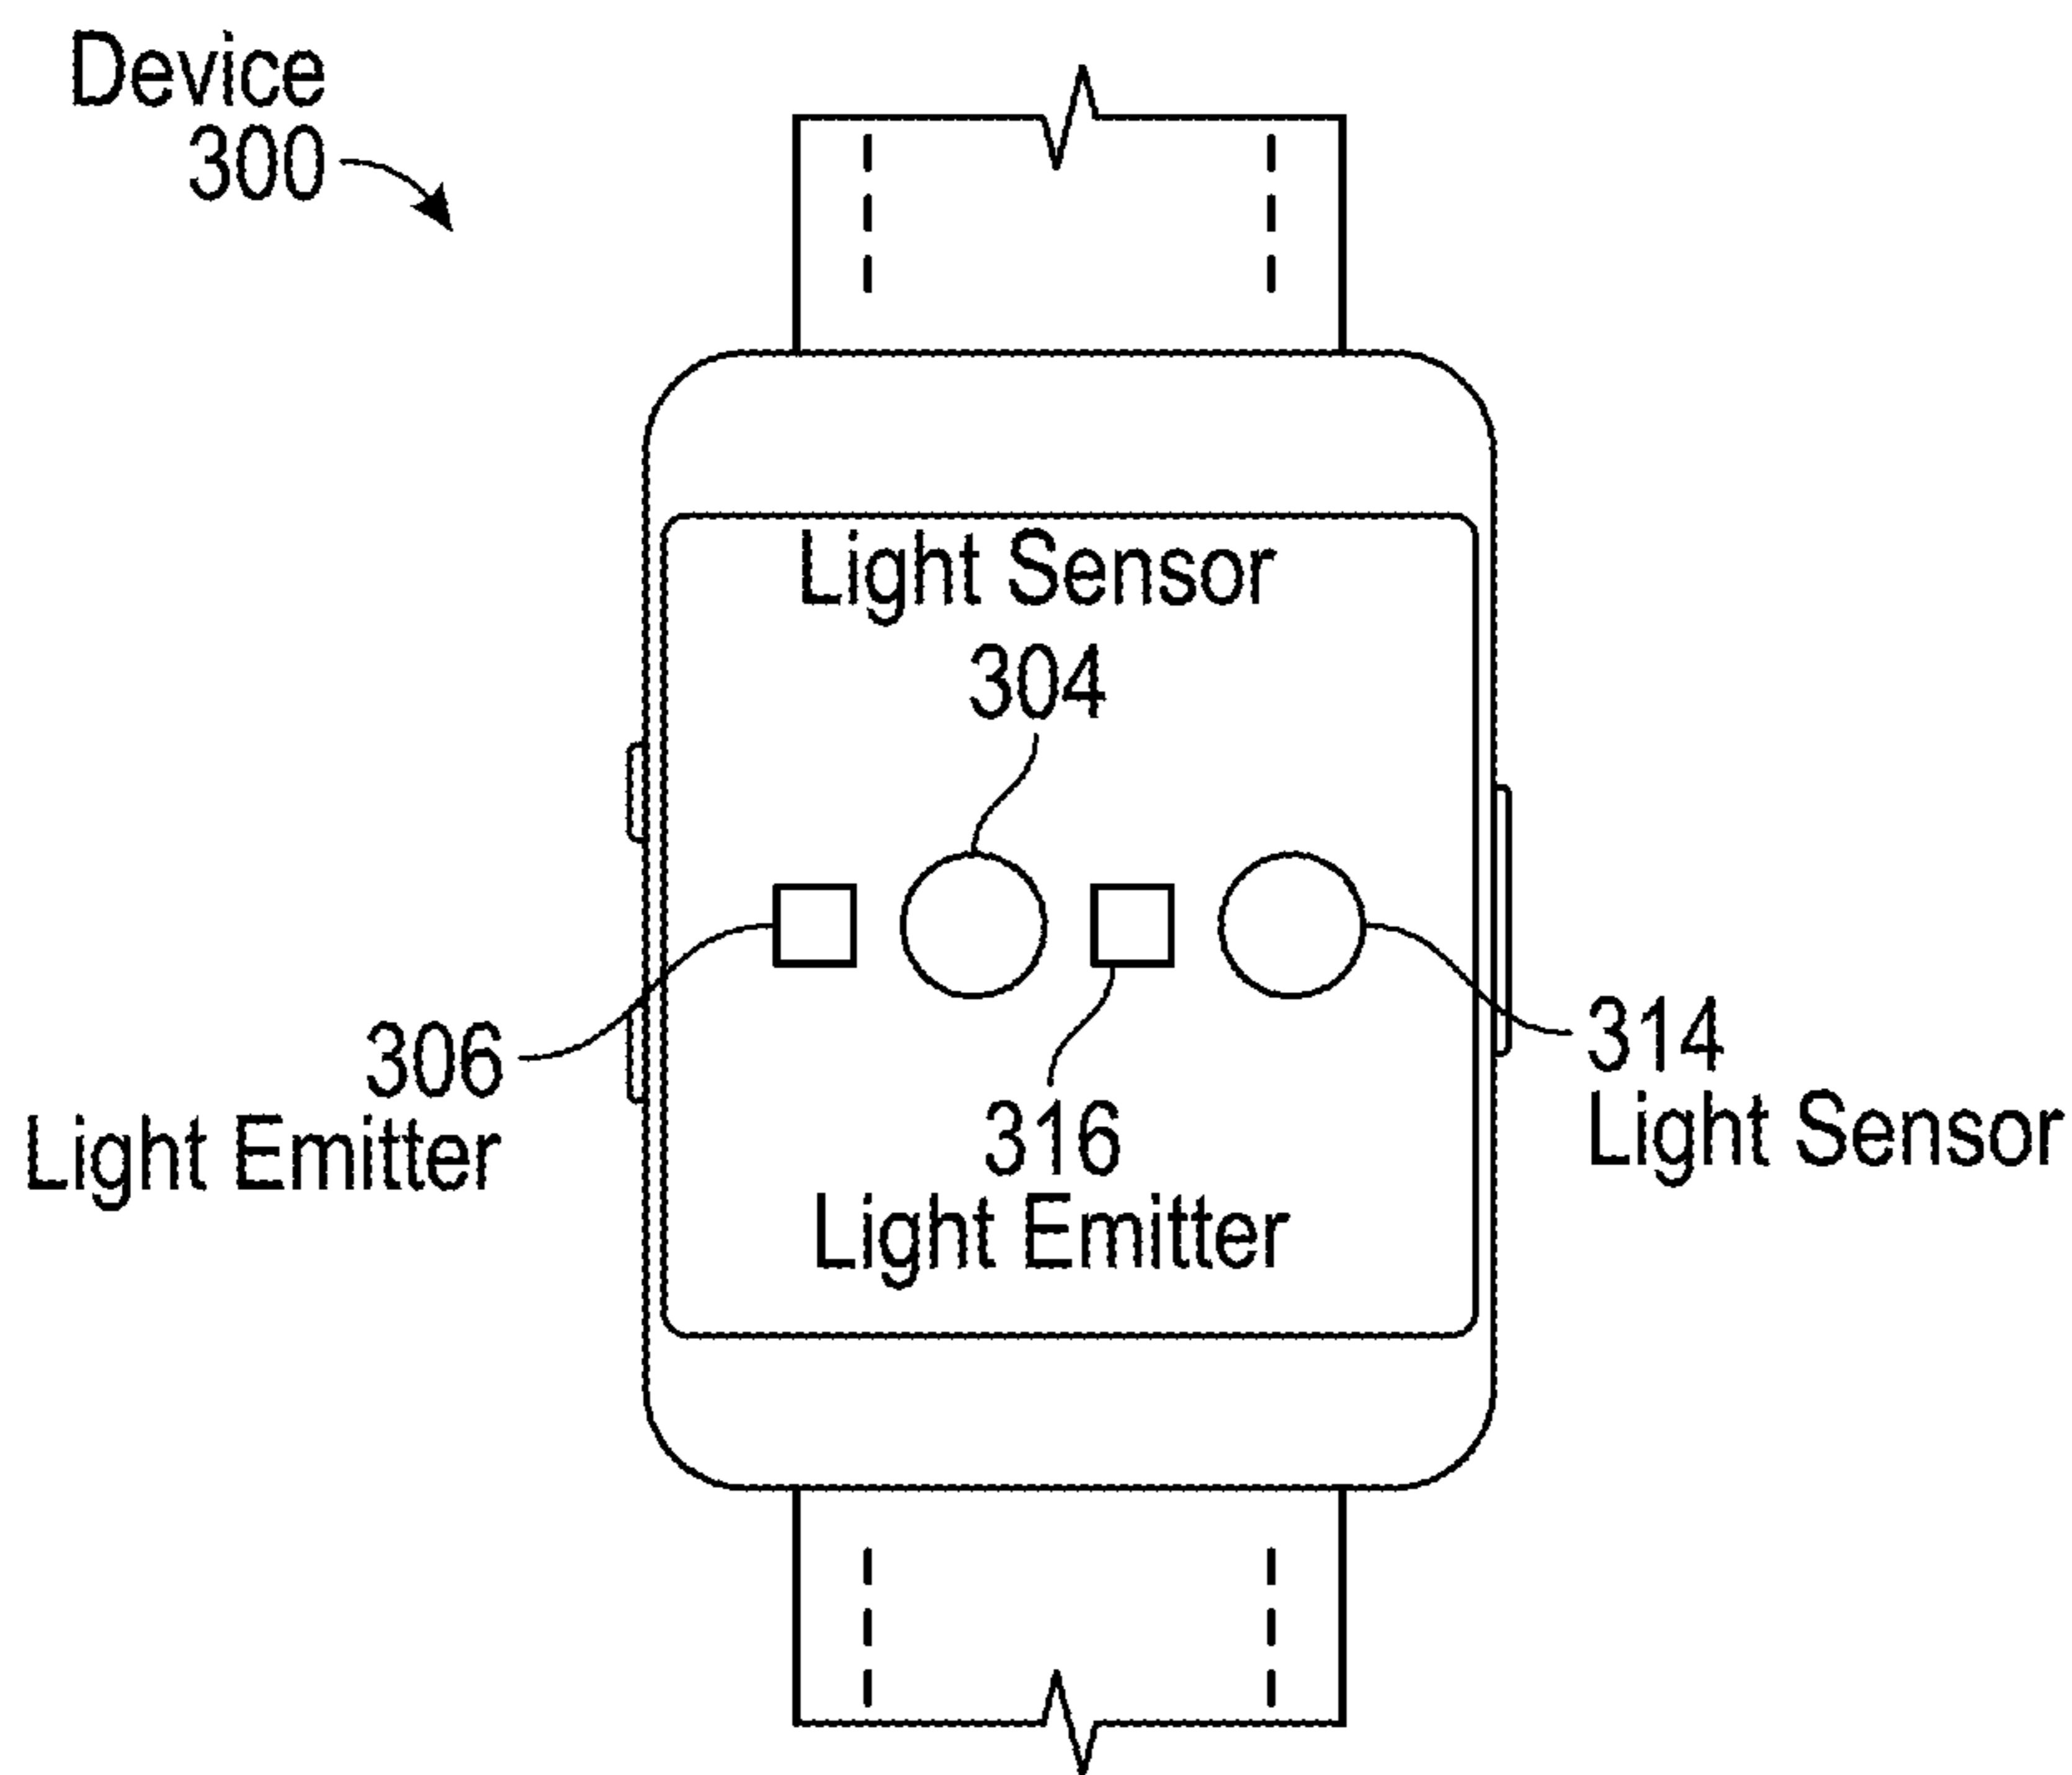


FIG. 3A

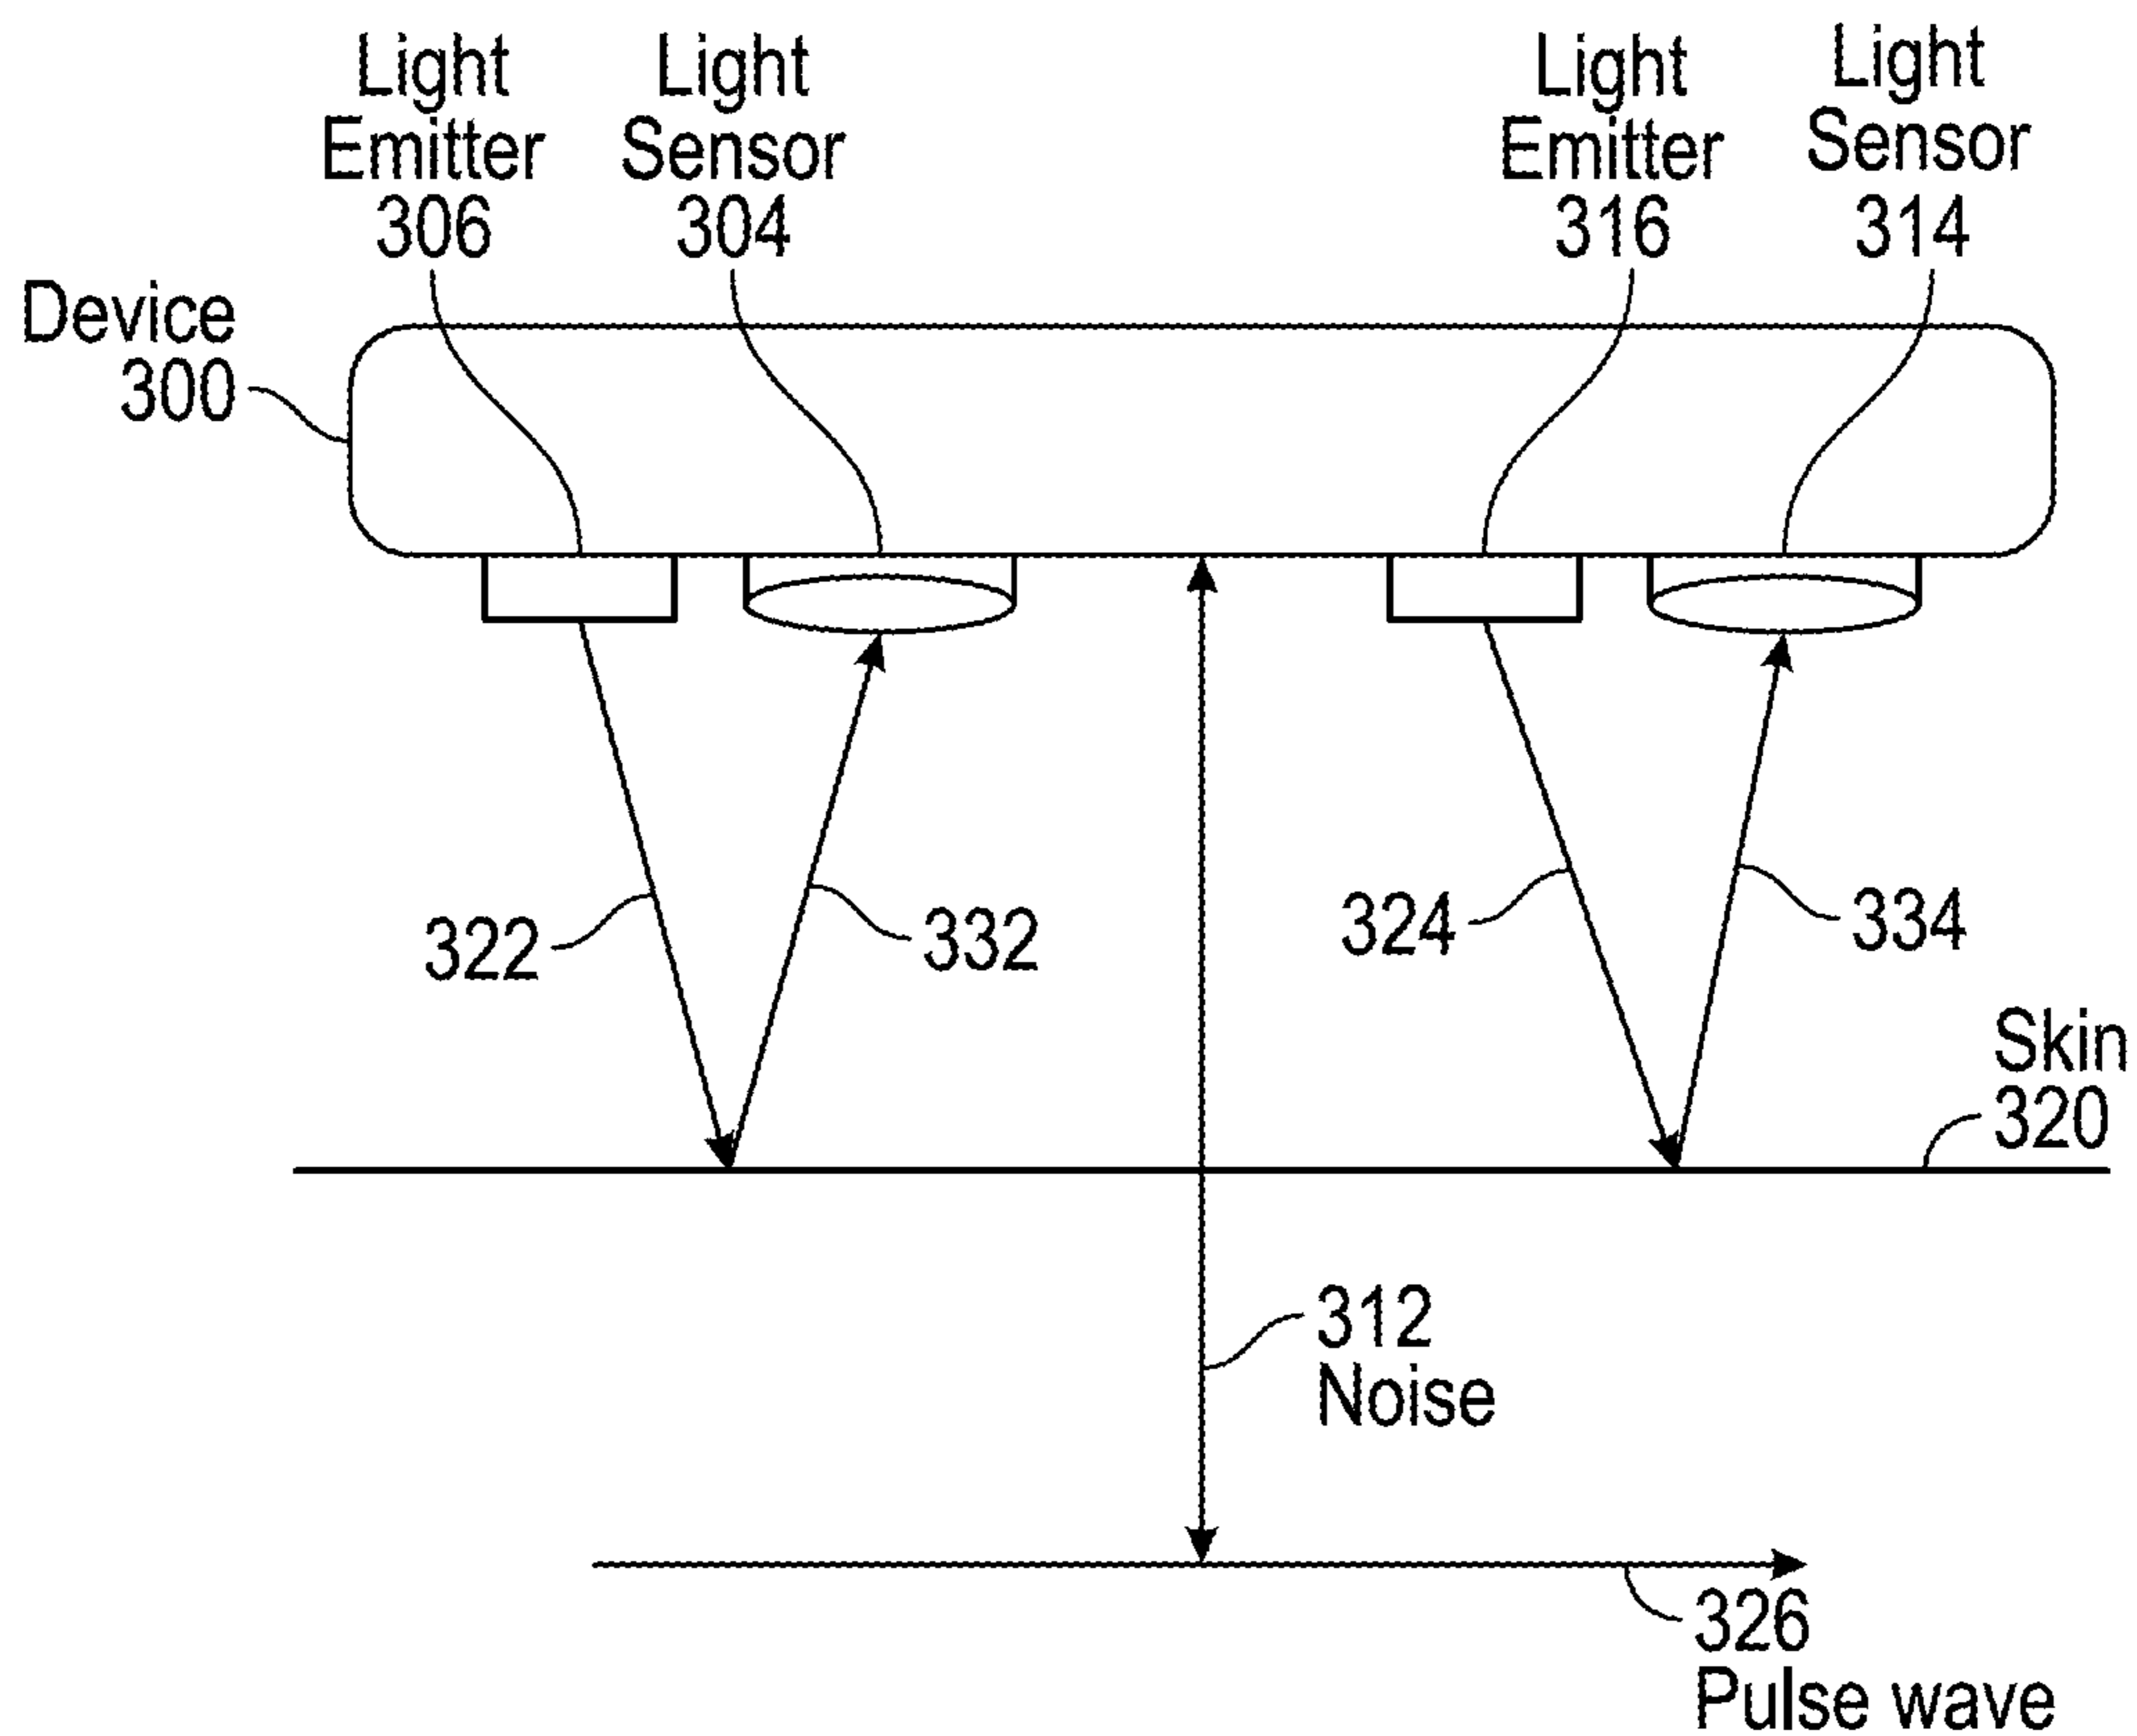


FIG. 3B

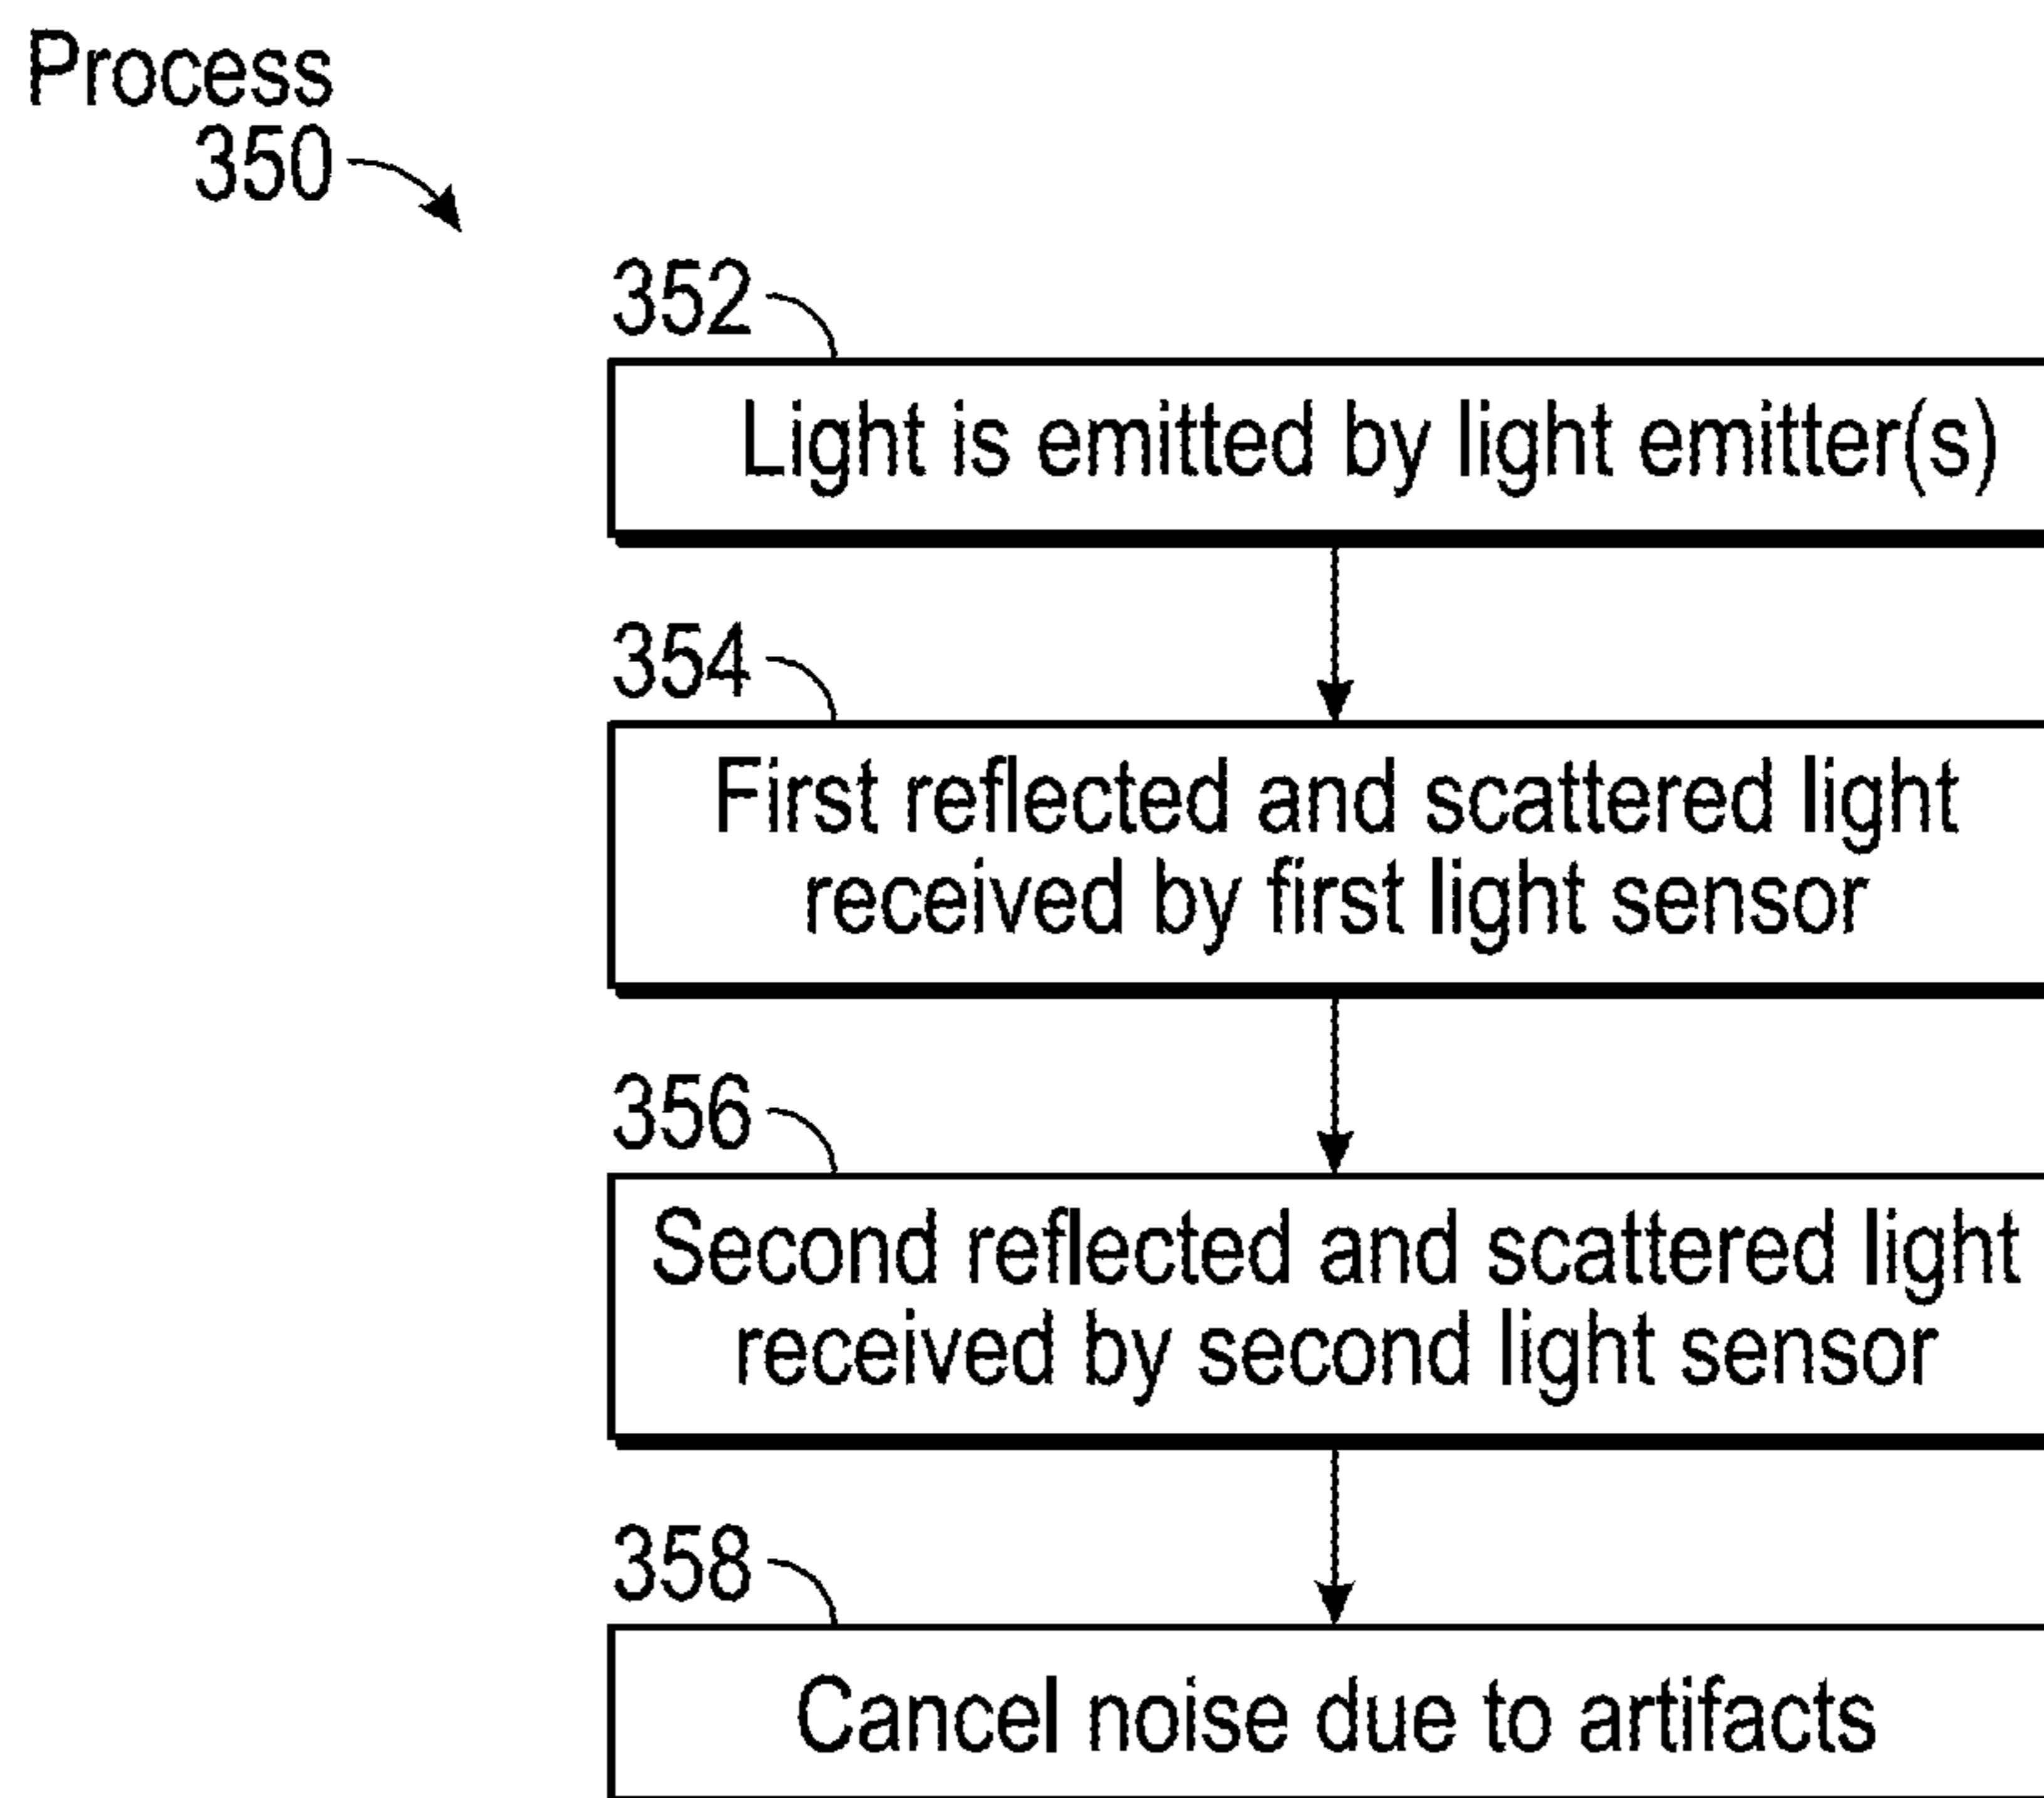


FIG. 3C

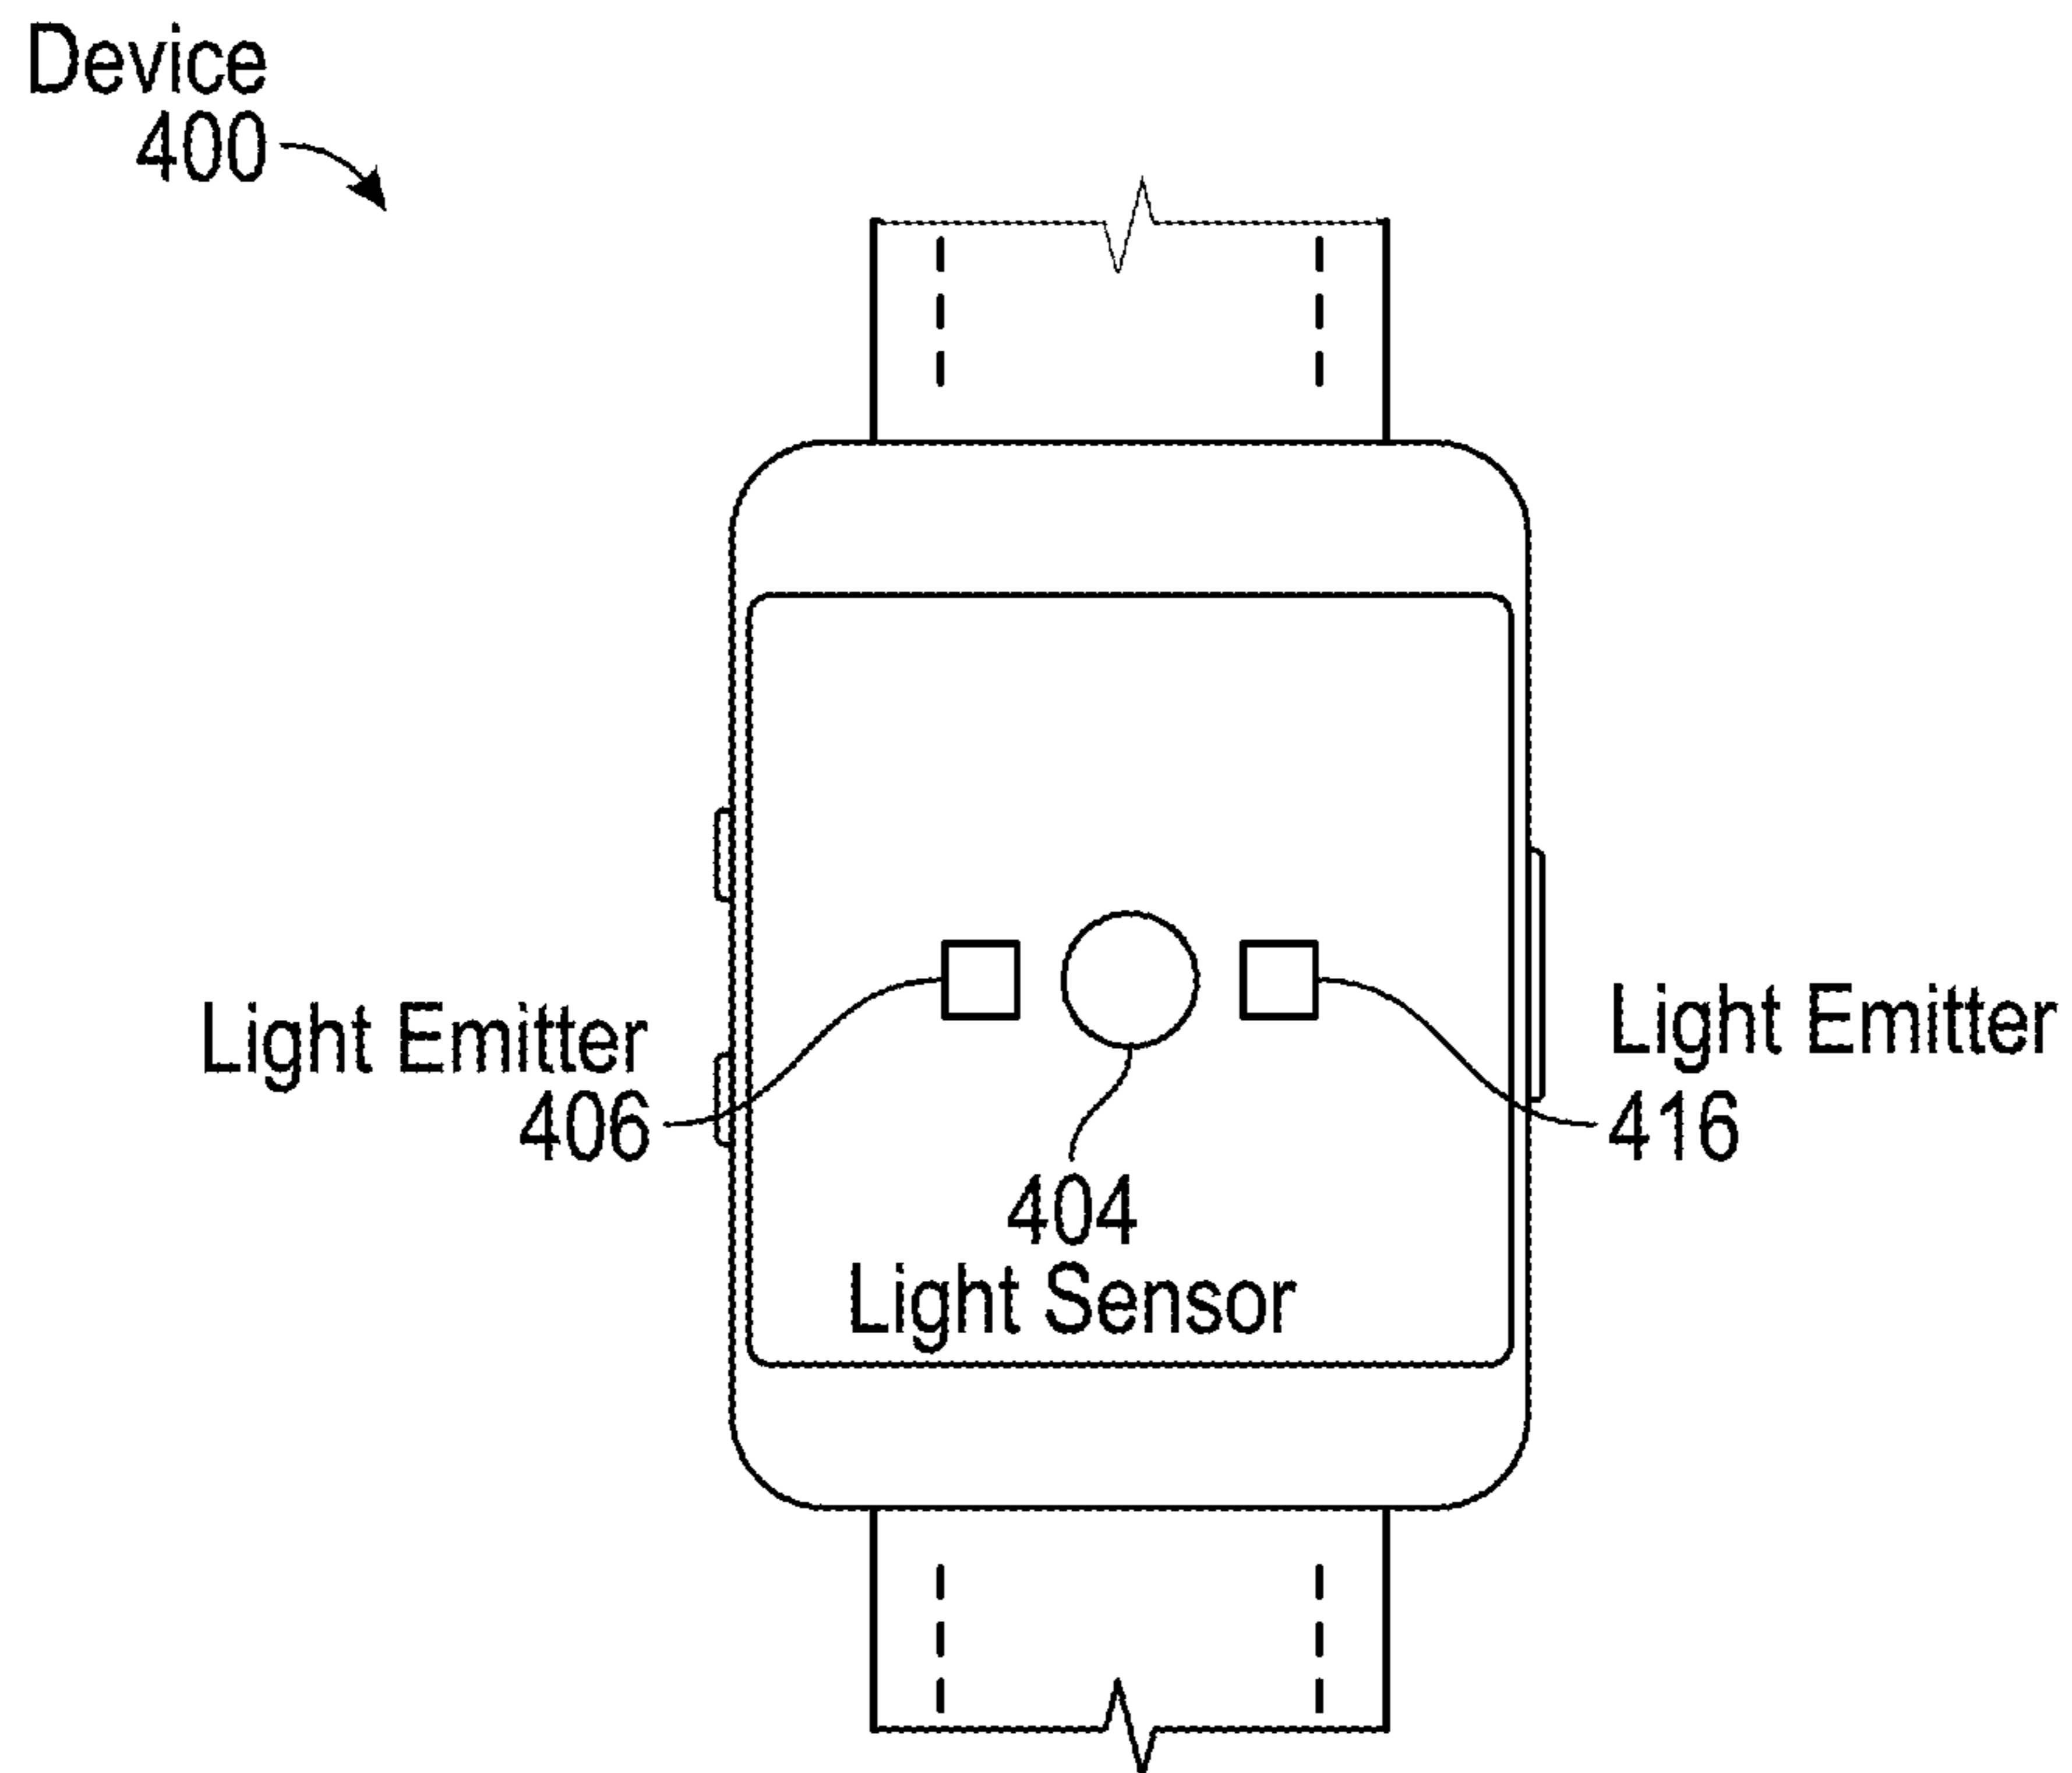


FIG. 4A

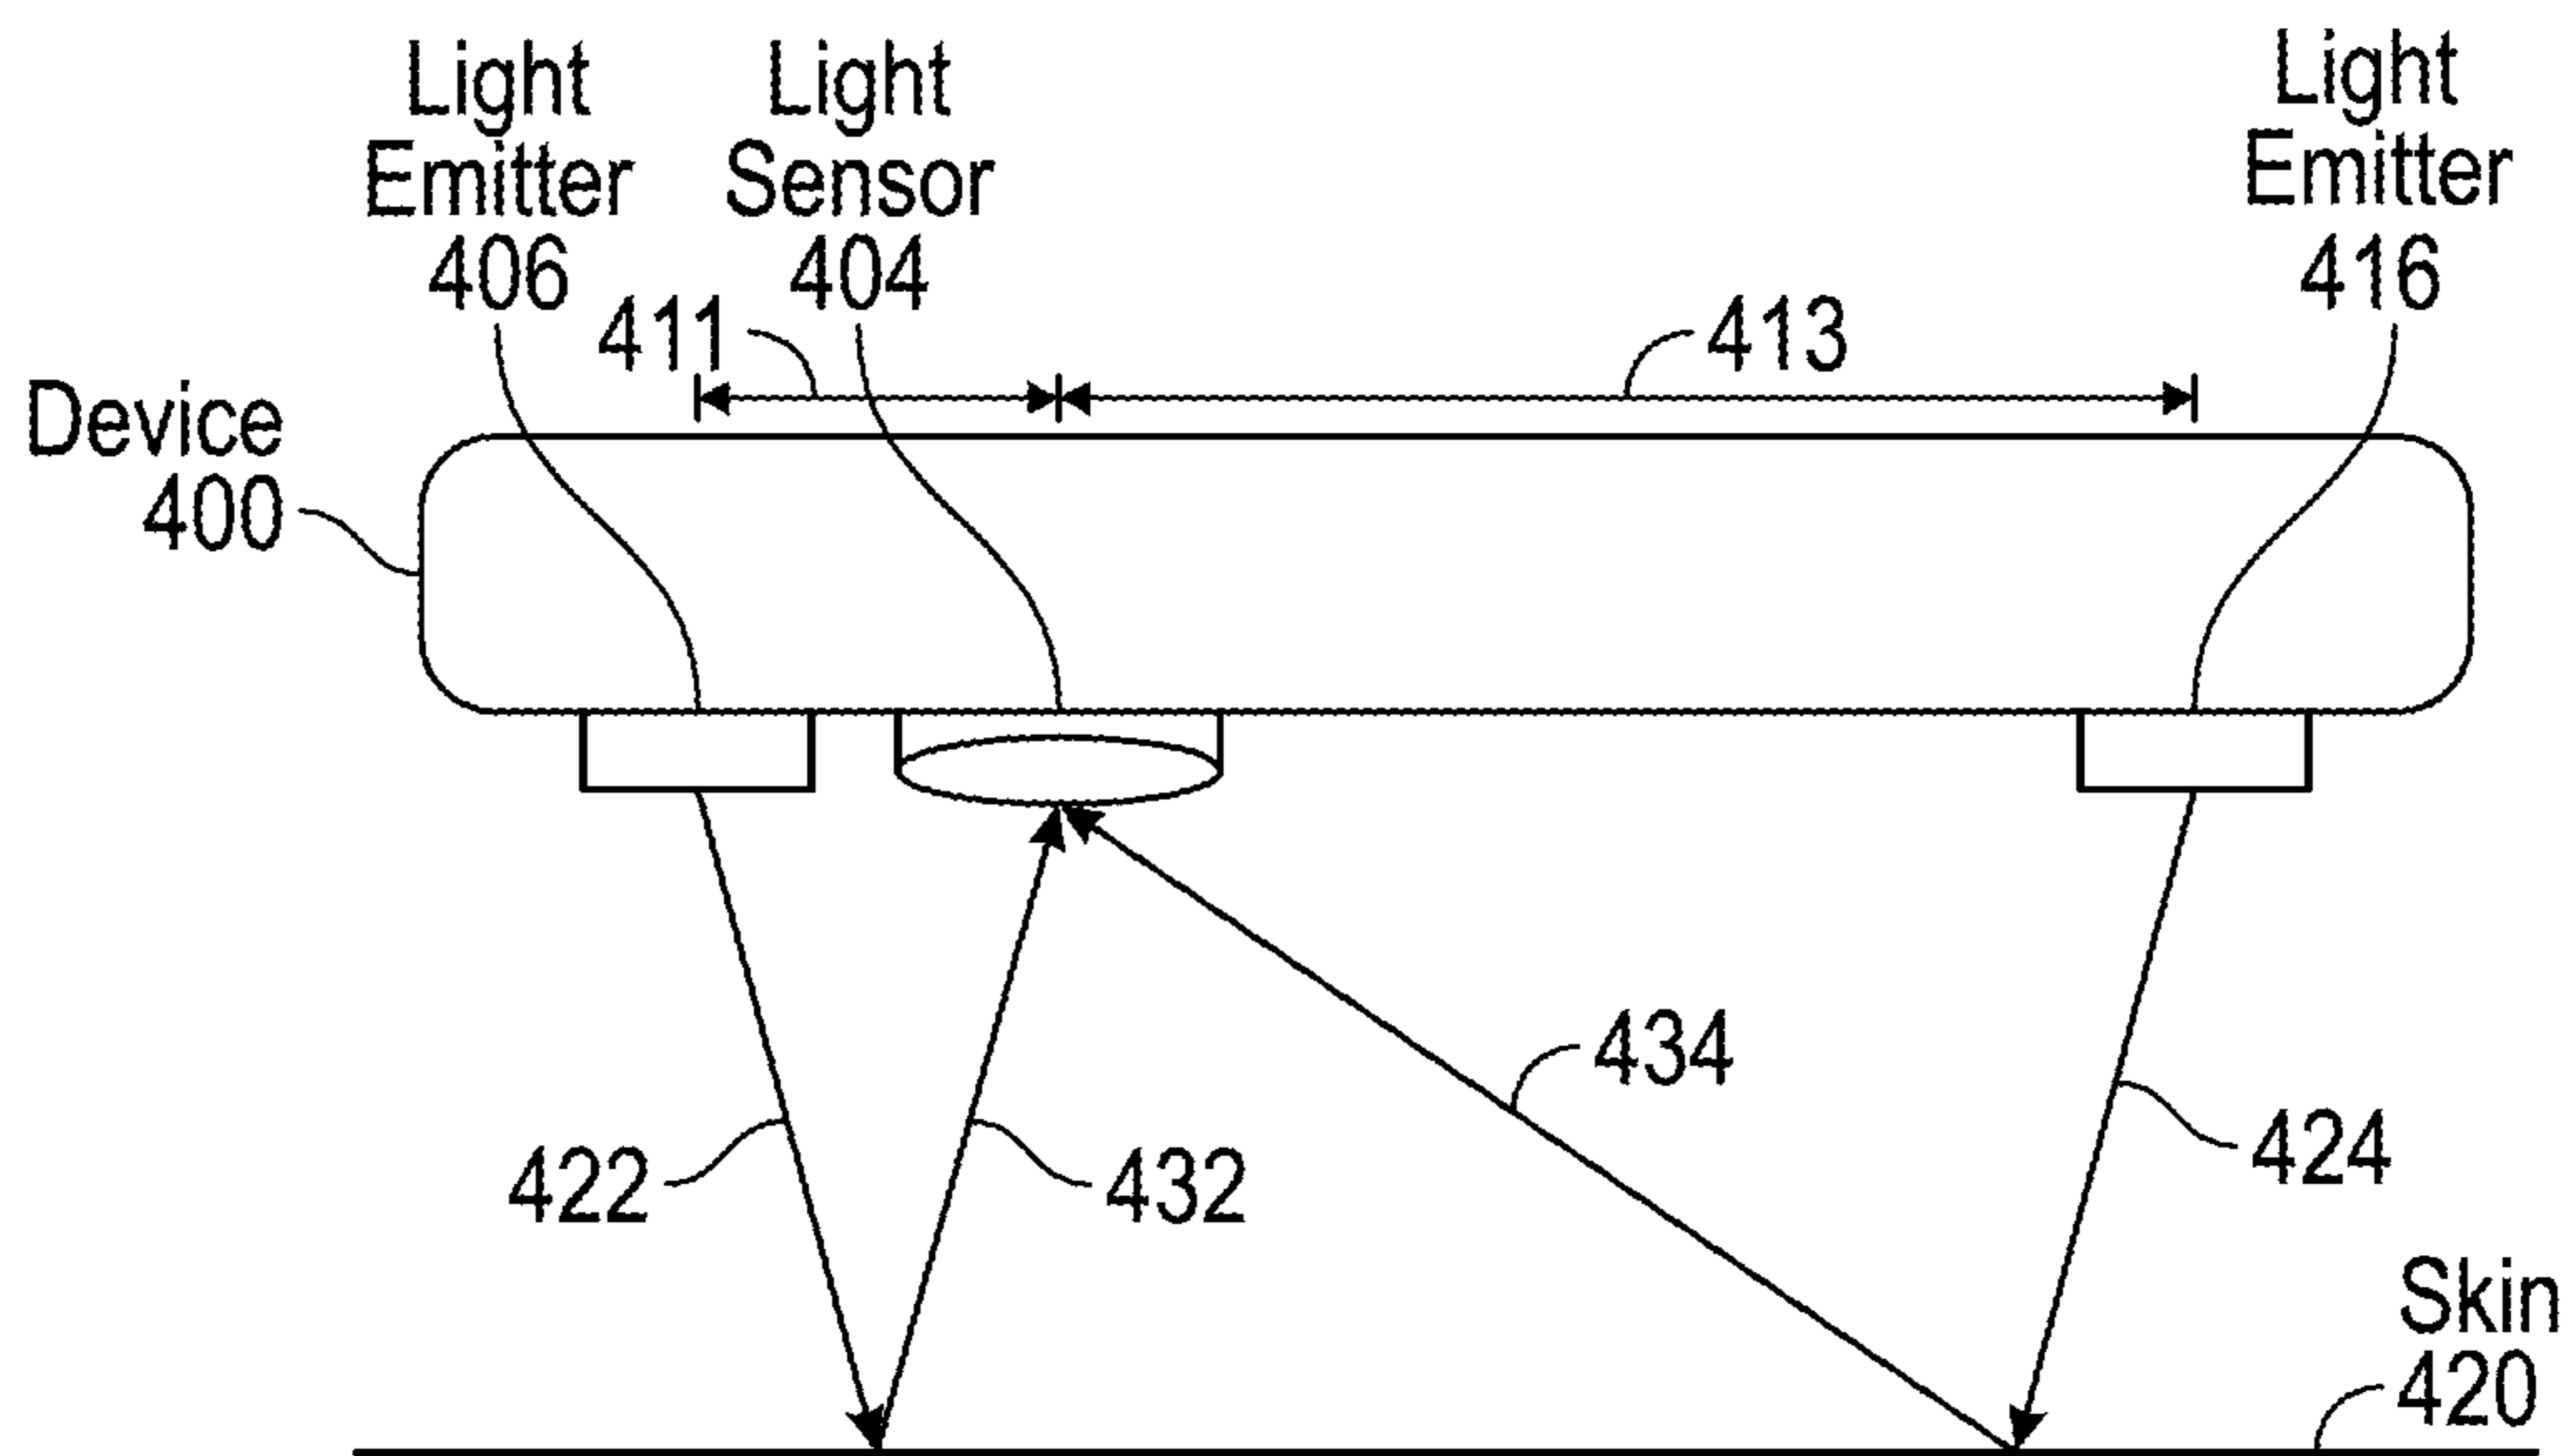


FIG. 4B

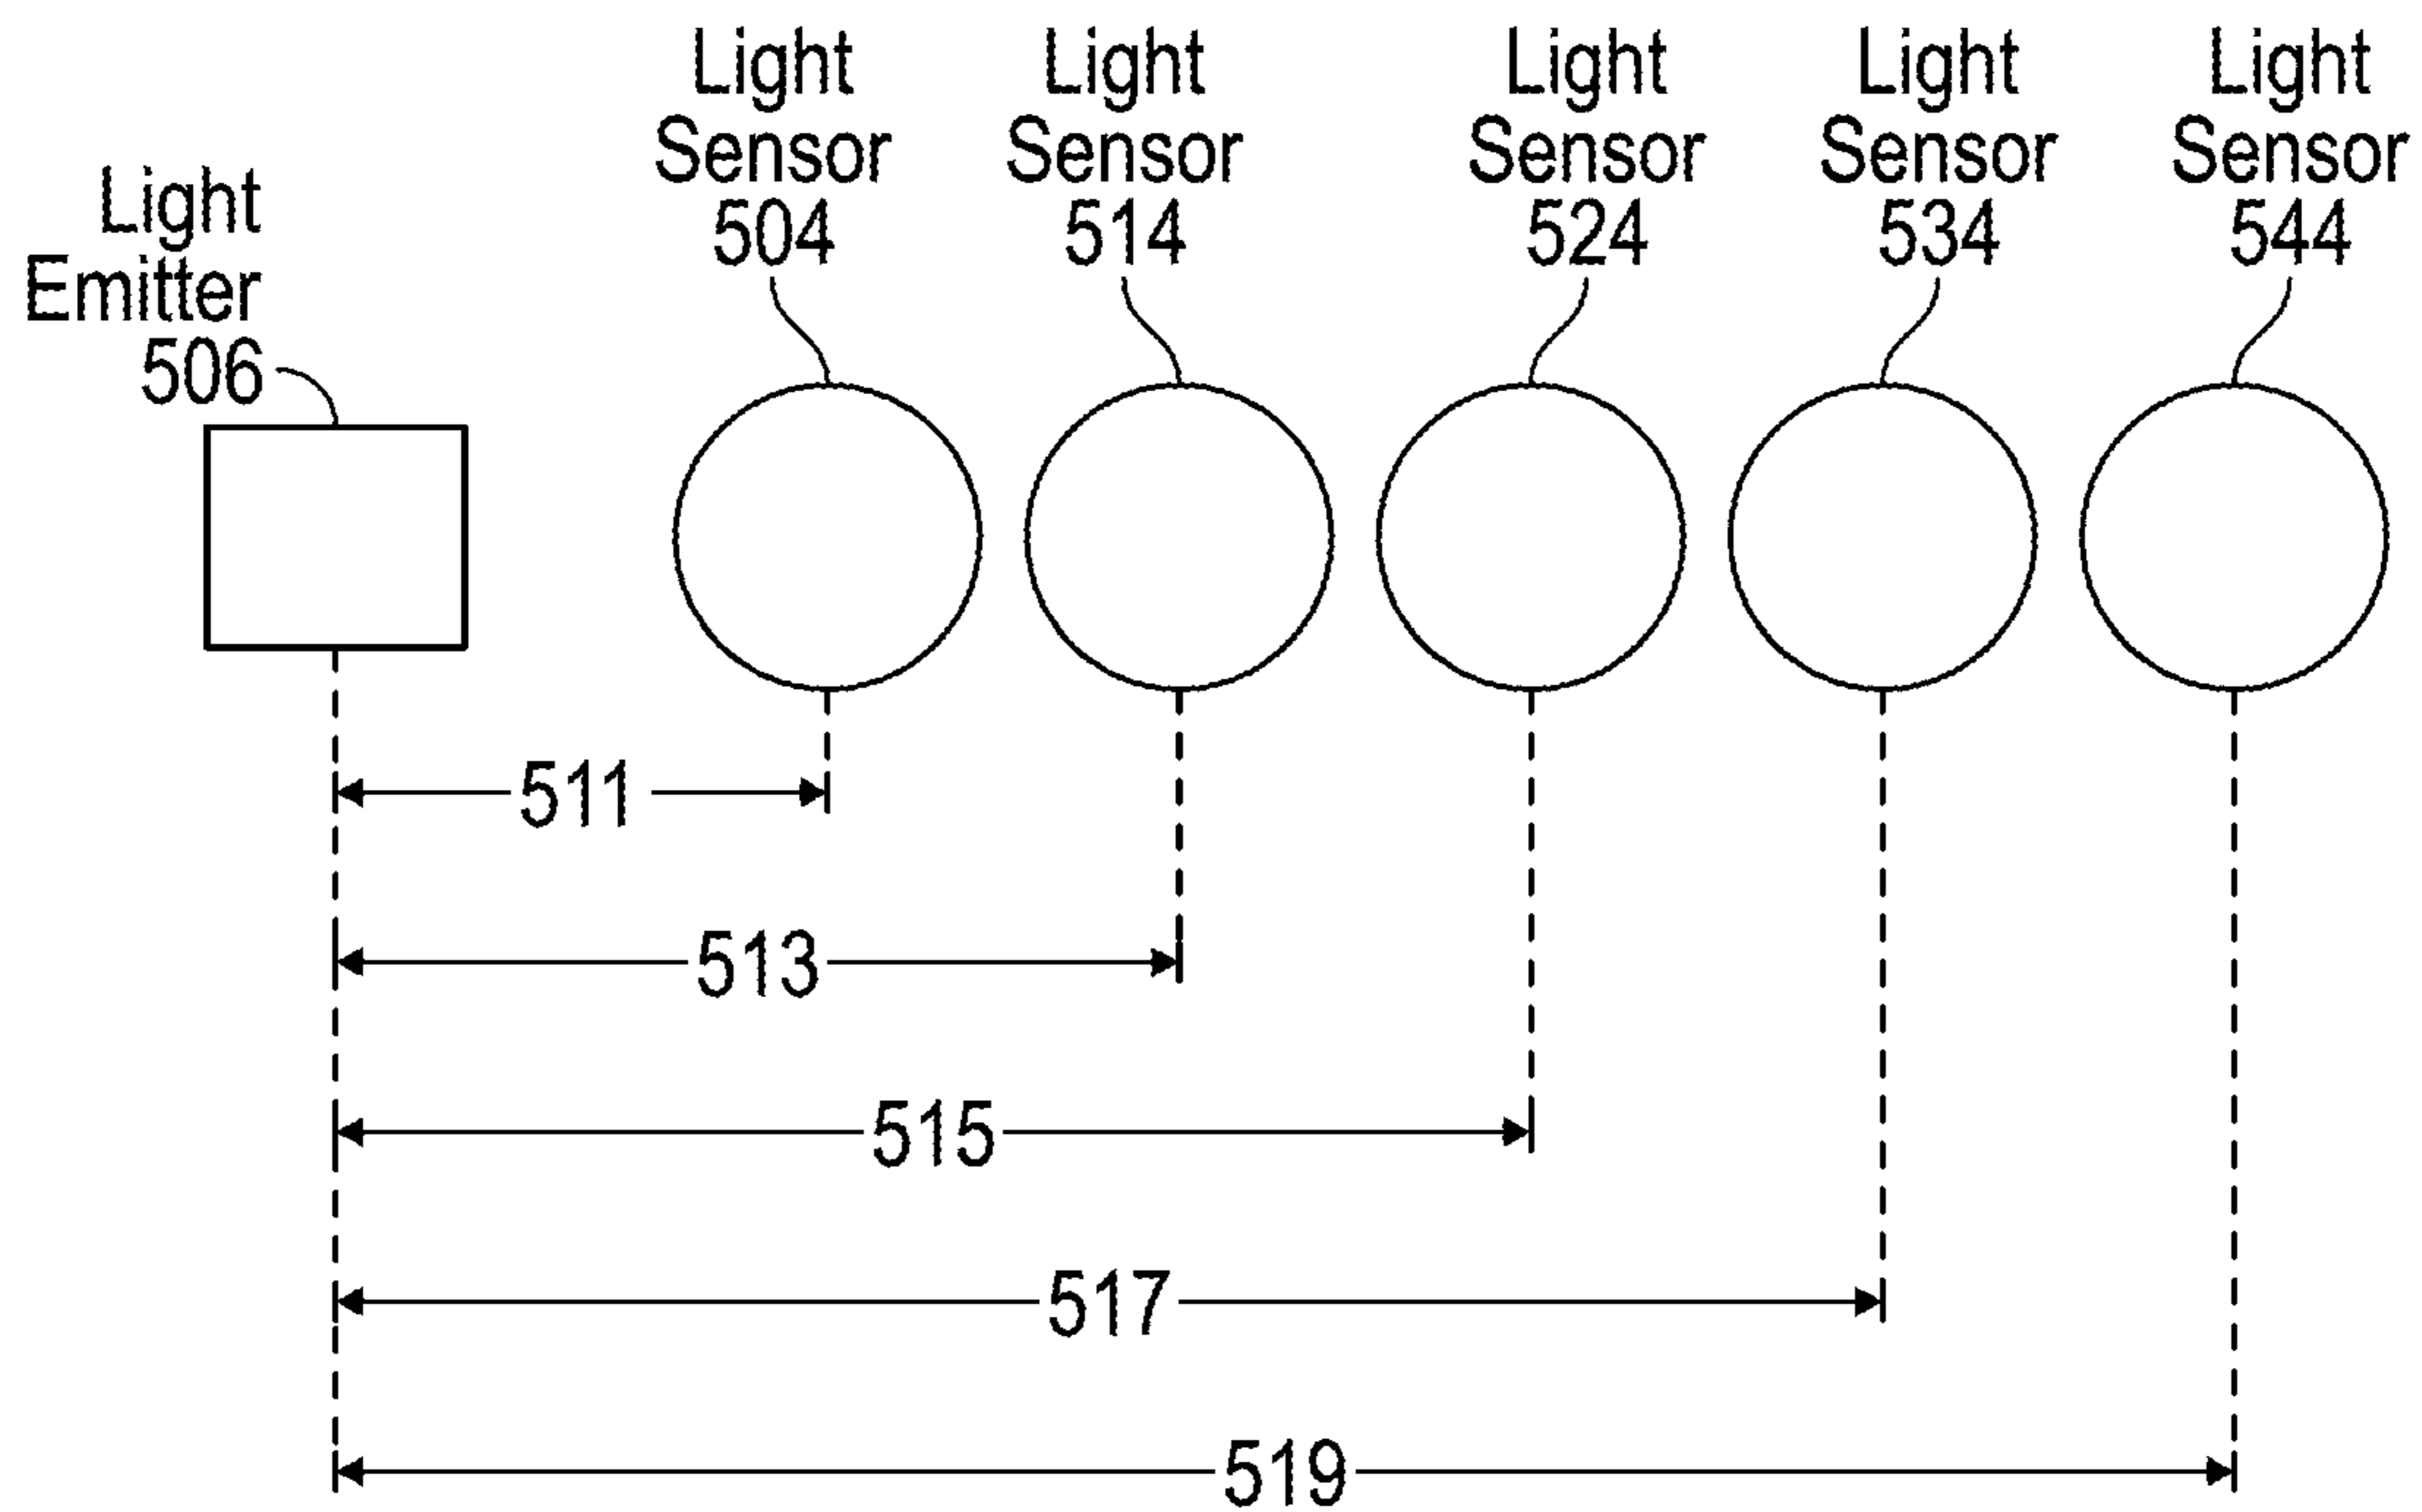


FIG. 5A

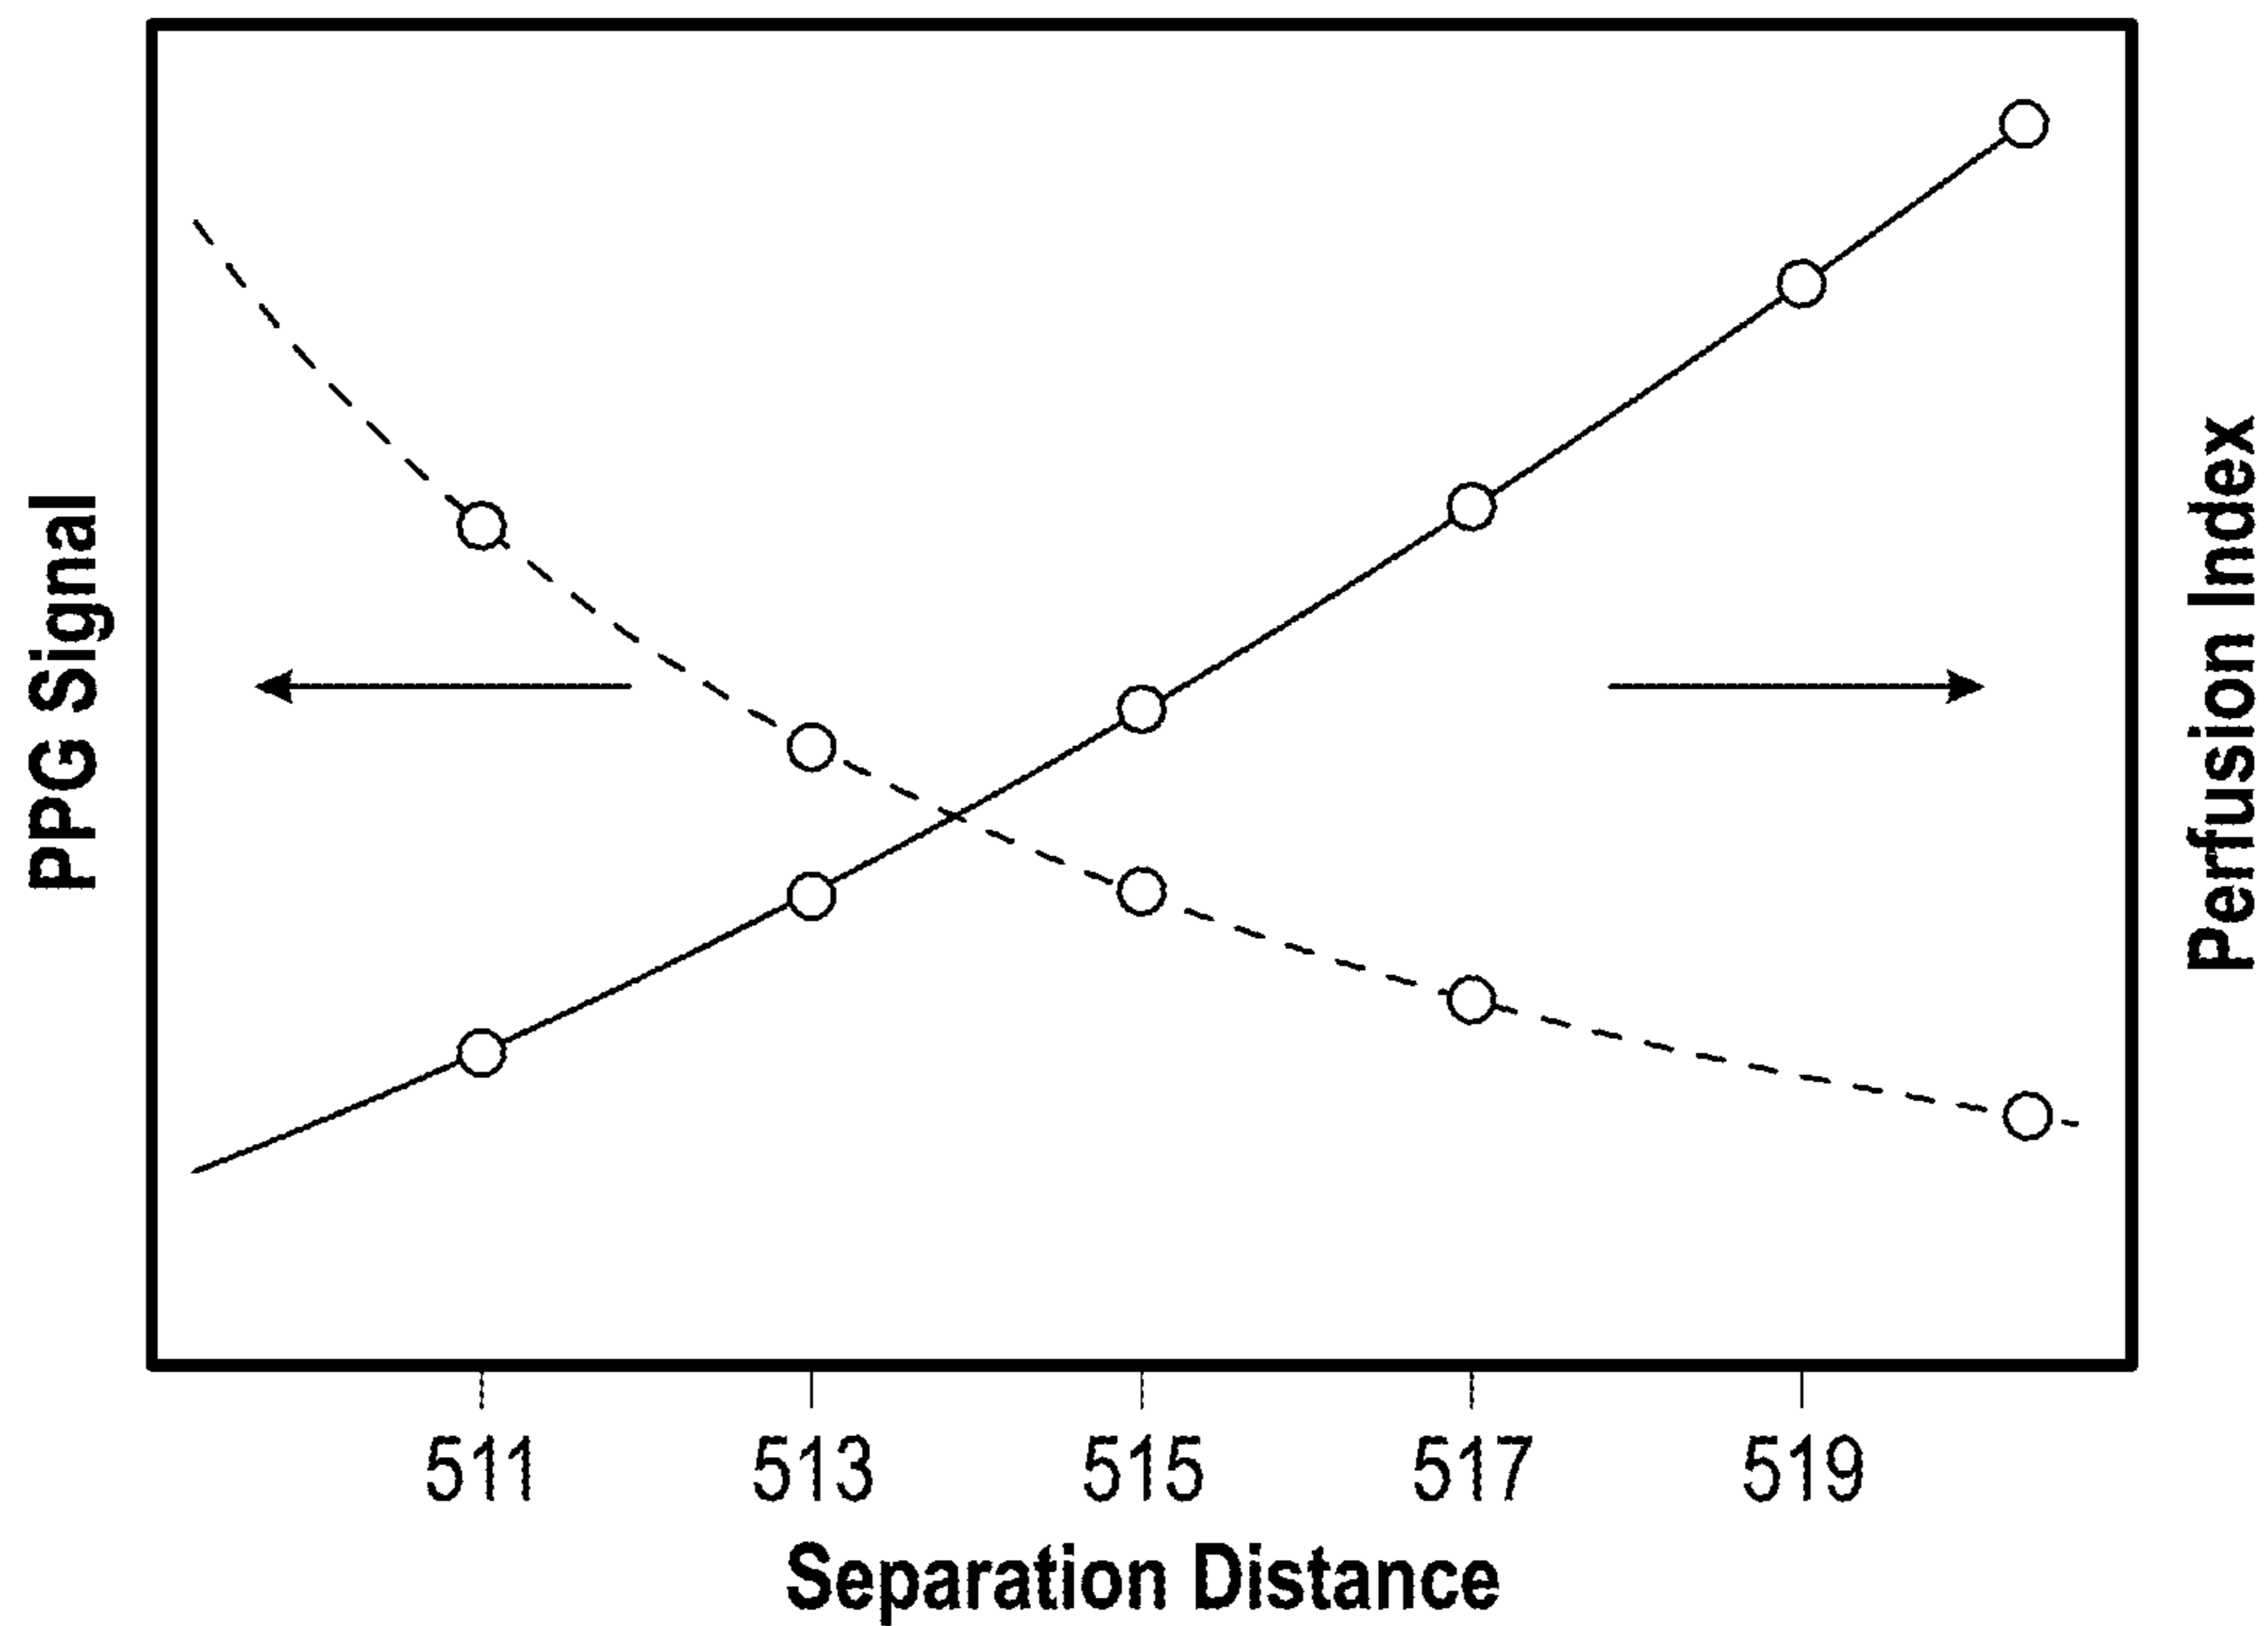


FIG. 5B



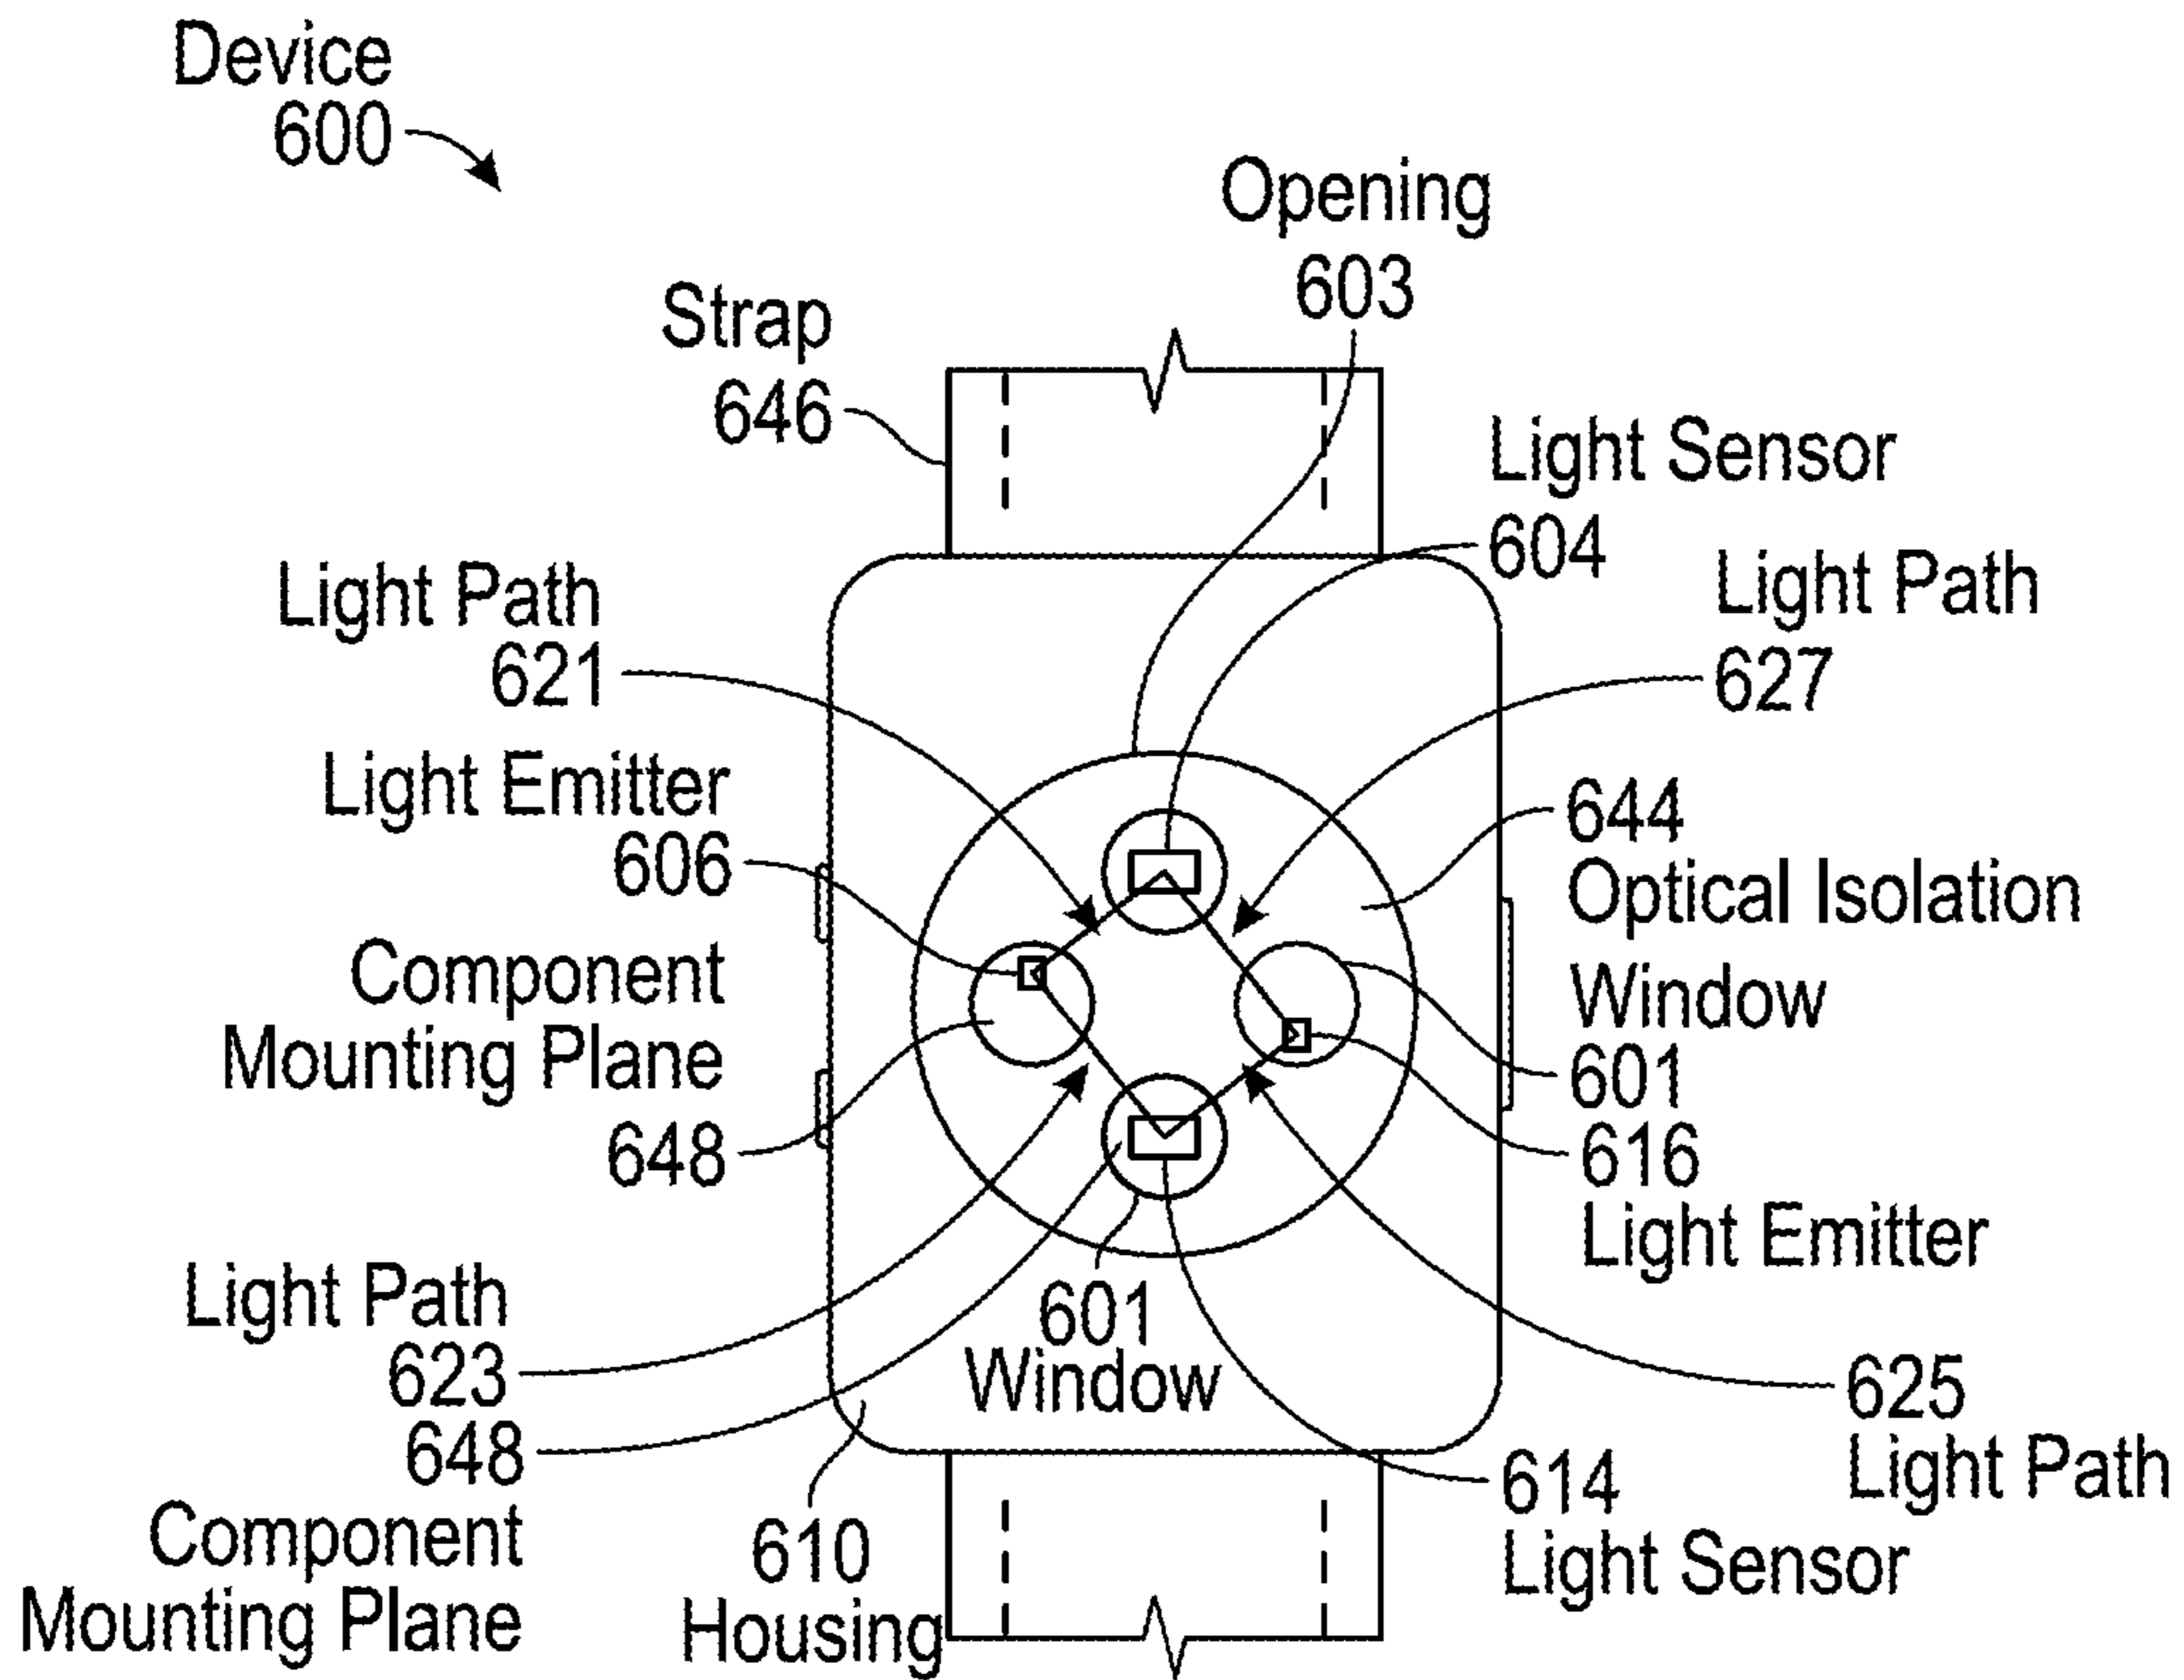


FIG. 6A

Light Path	Light Emitter	Light Sensor	Path Length (mm)	PPG Signal	Perfusion Index
625	616	614	4.944	1.11	0.96
621	606	604	5.444	0.75	1.10
623	606	614	5.915	0.51	1.23
627	616	604	6.543	0.31	1.39

FIG. 6B

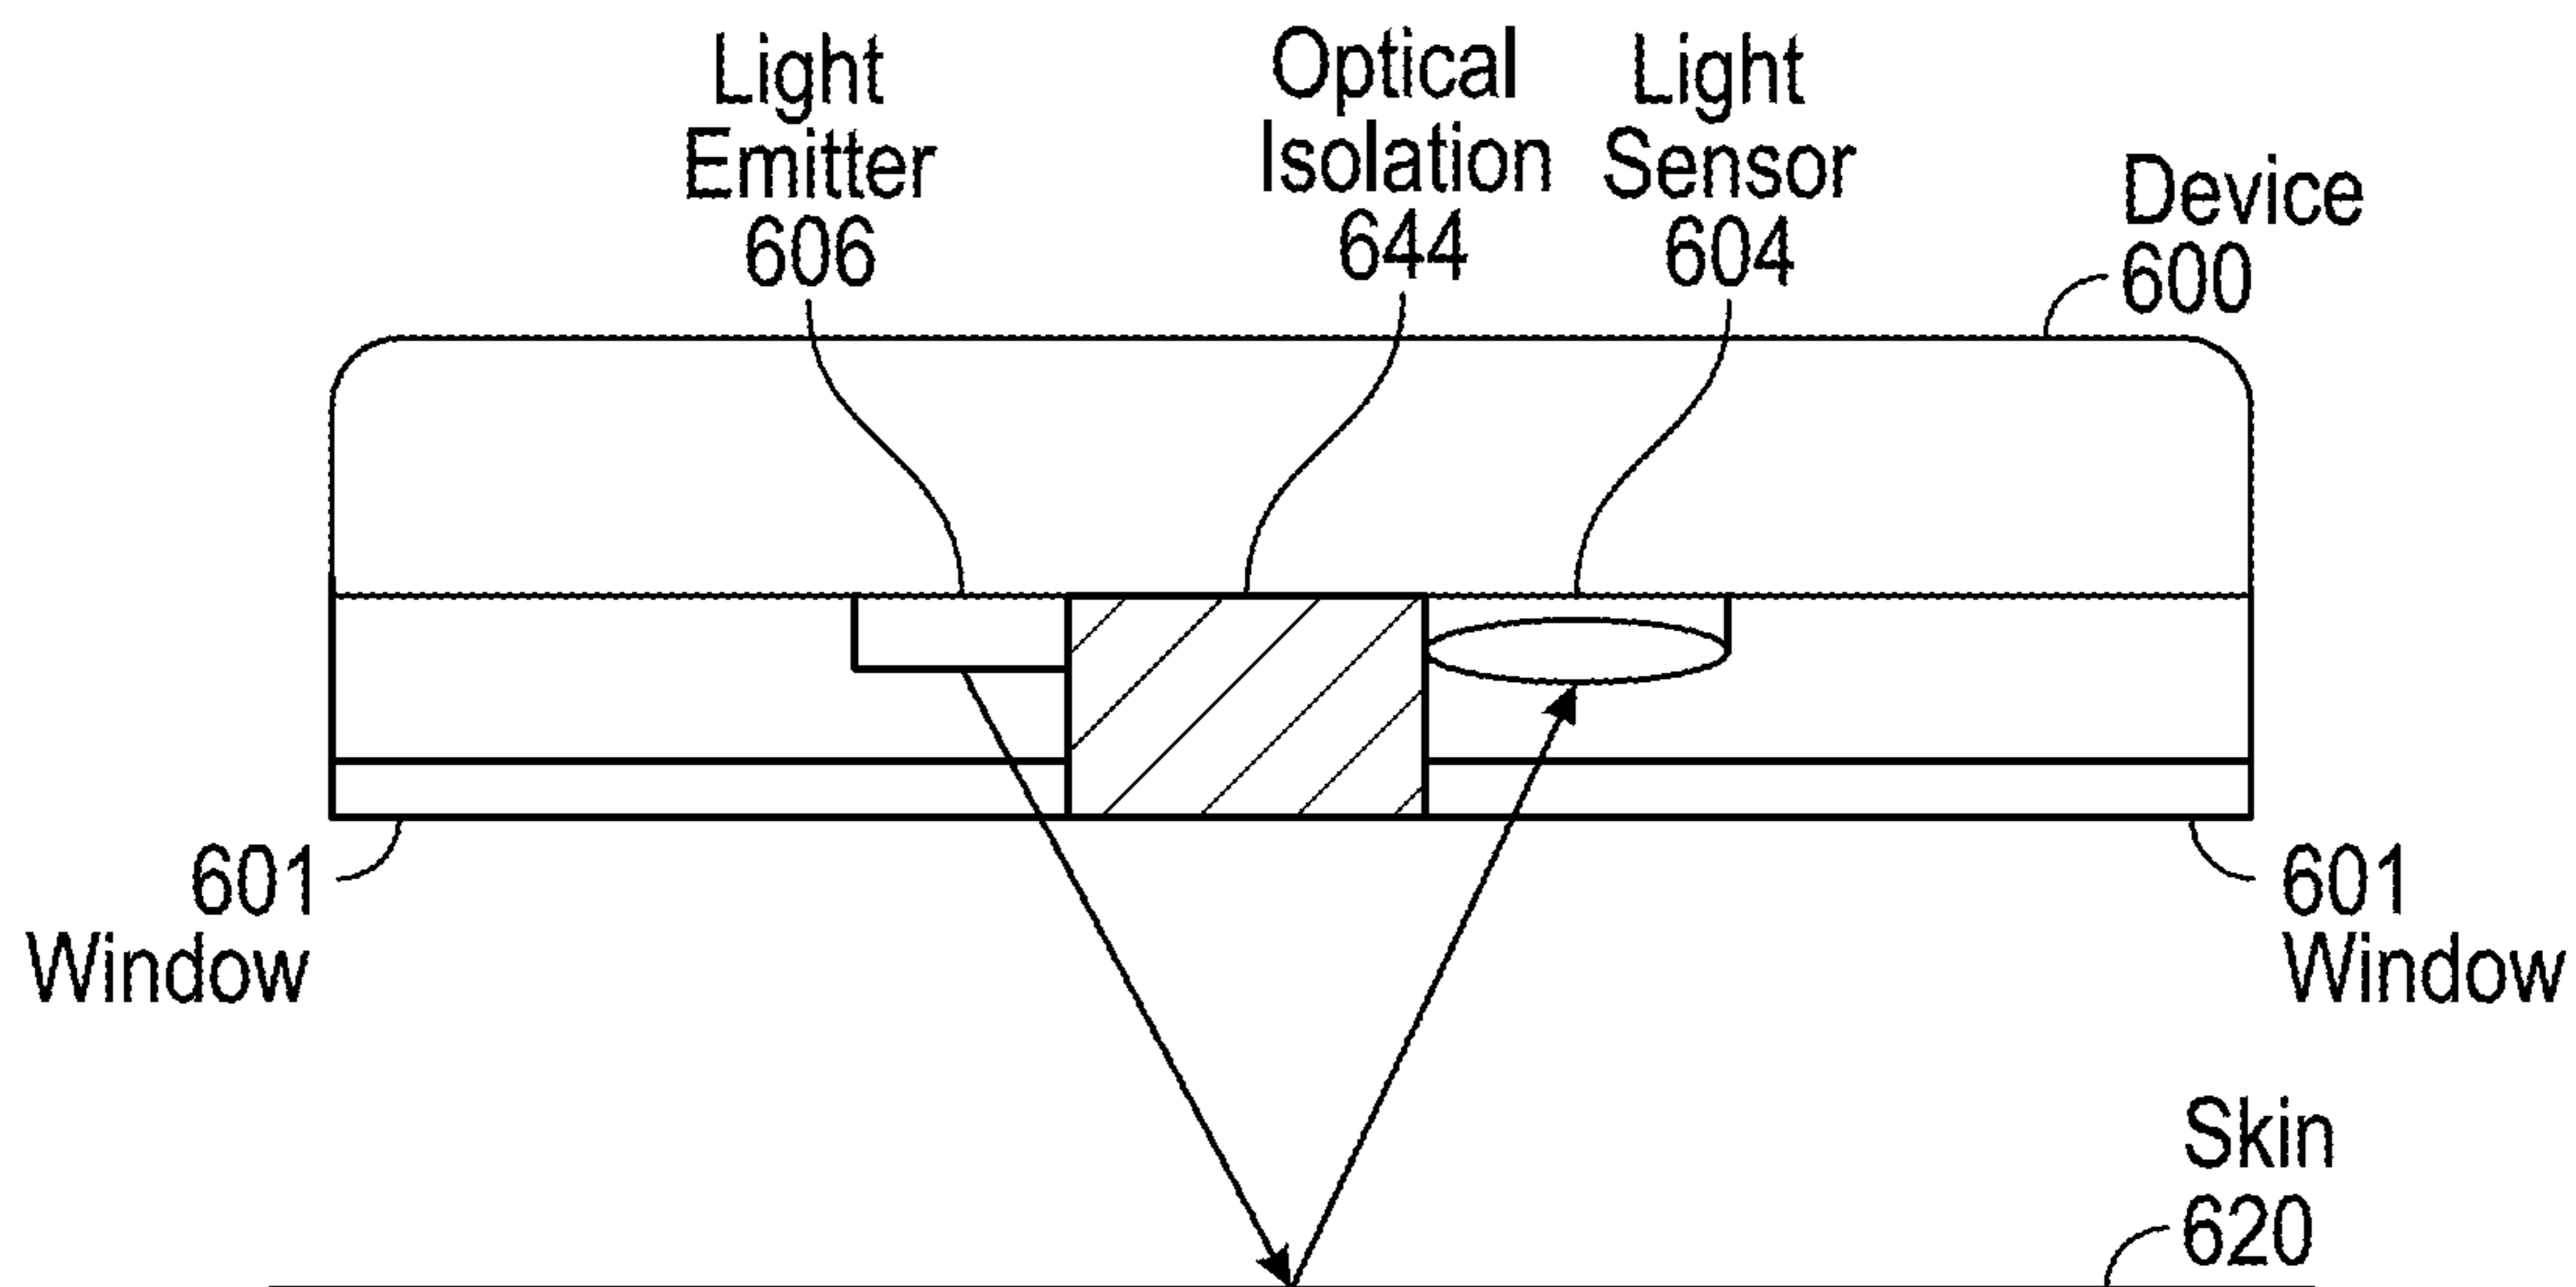


FIG. 6C

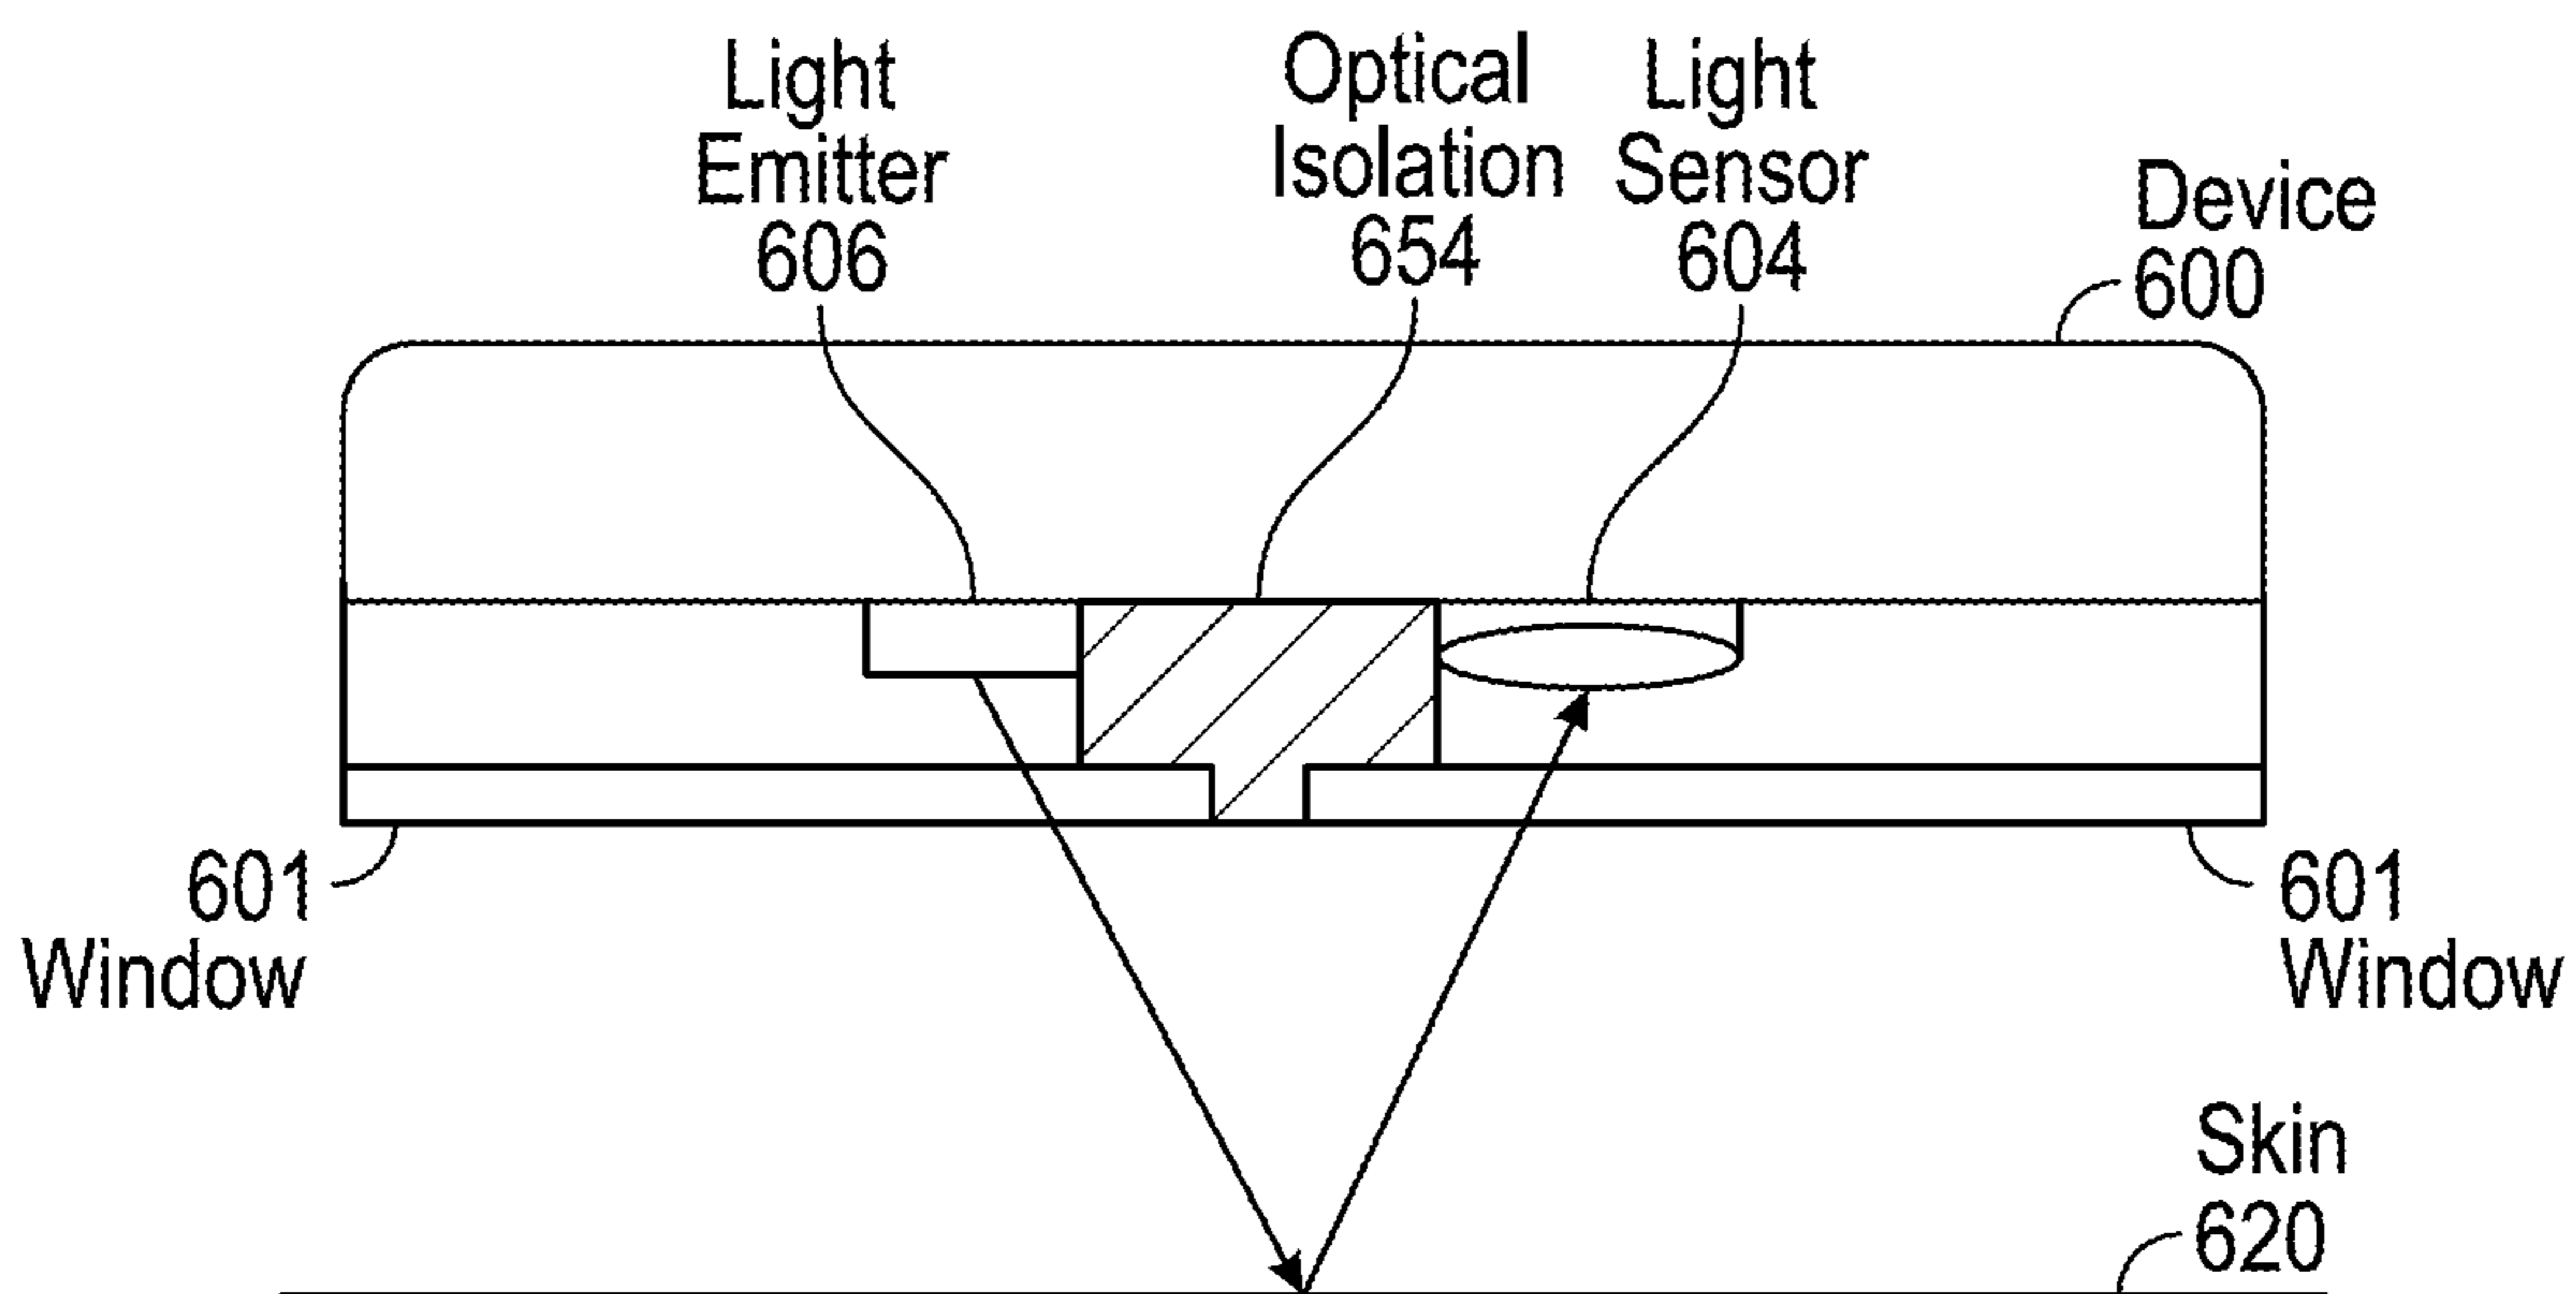


FIG. 6D

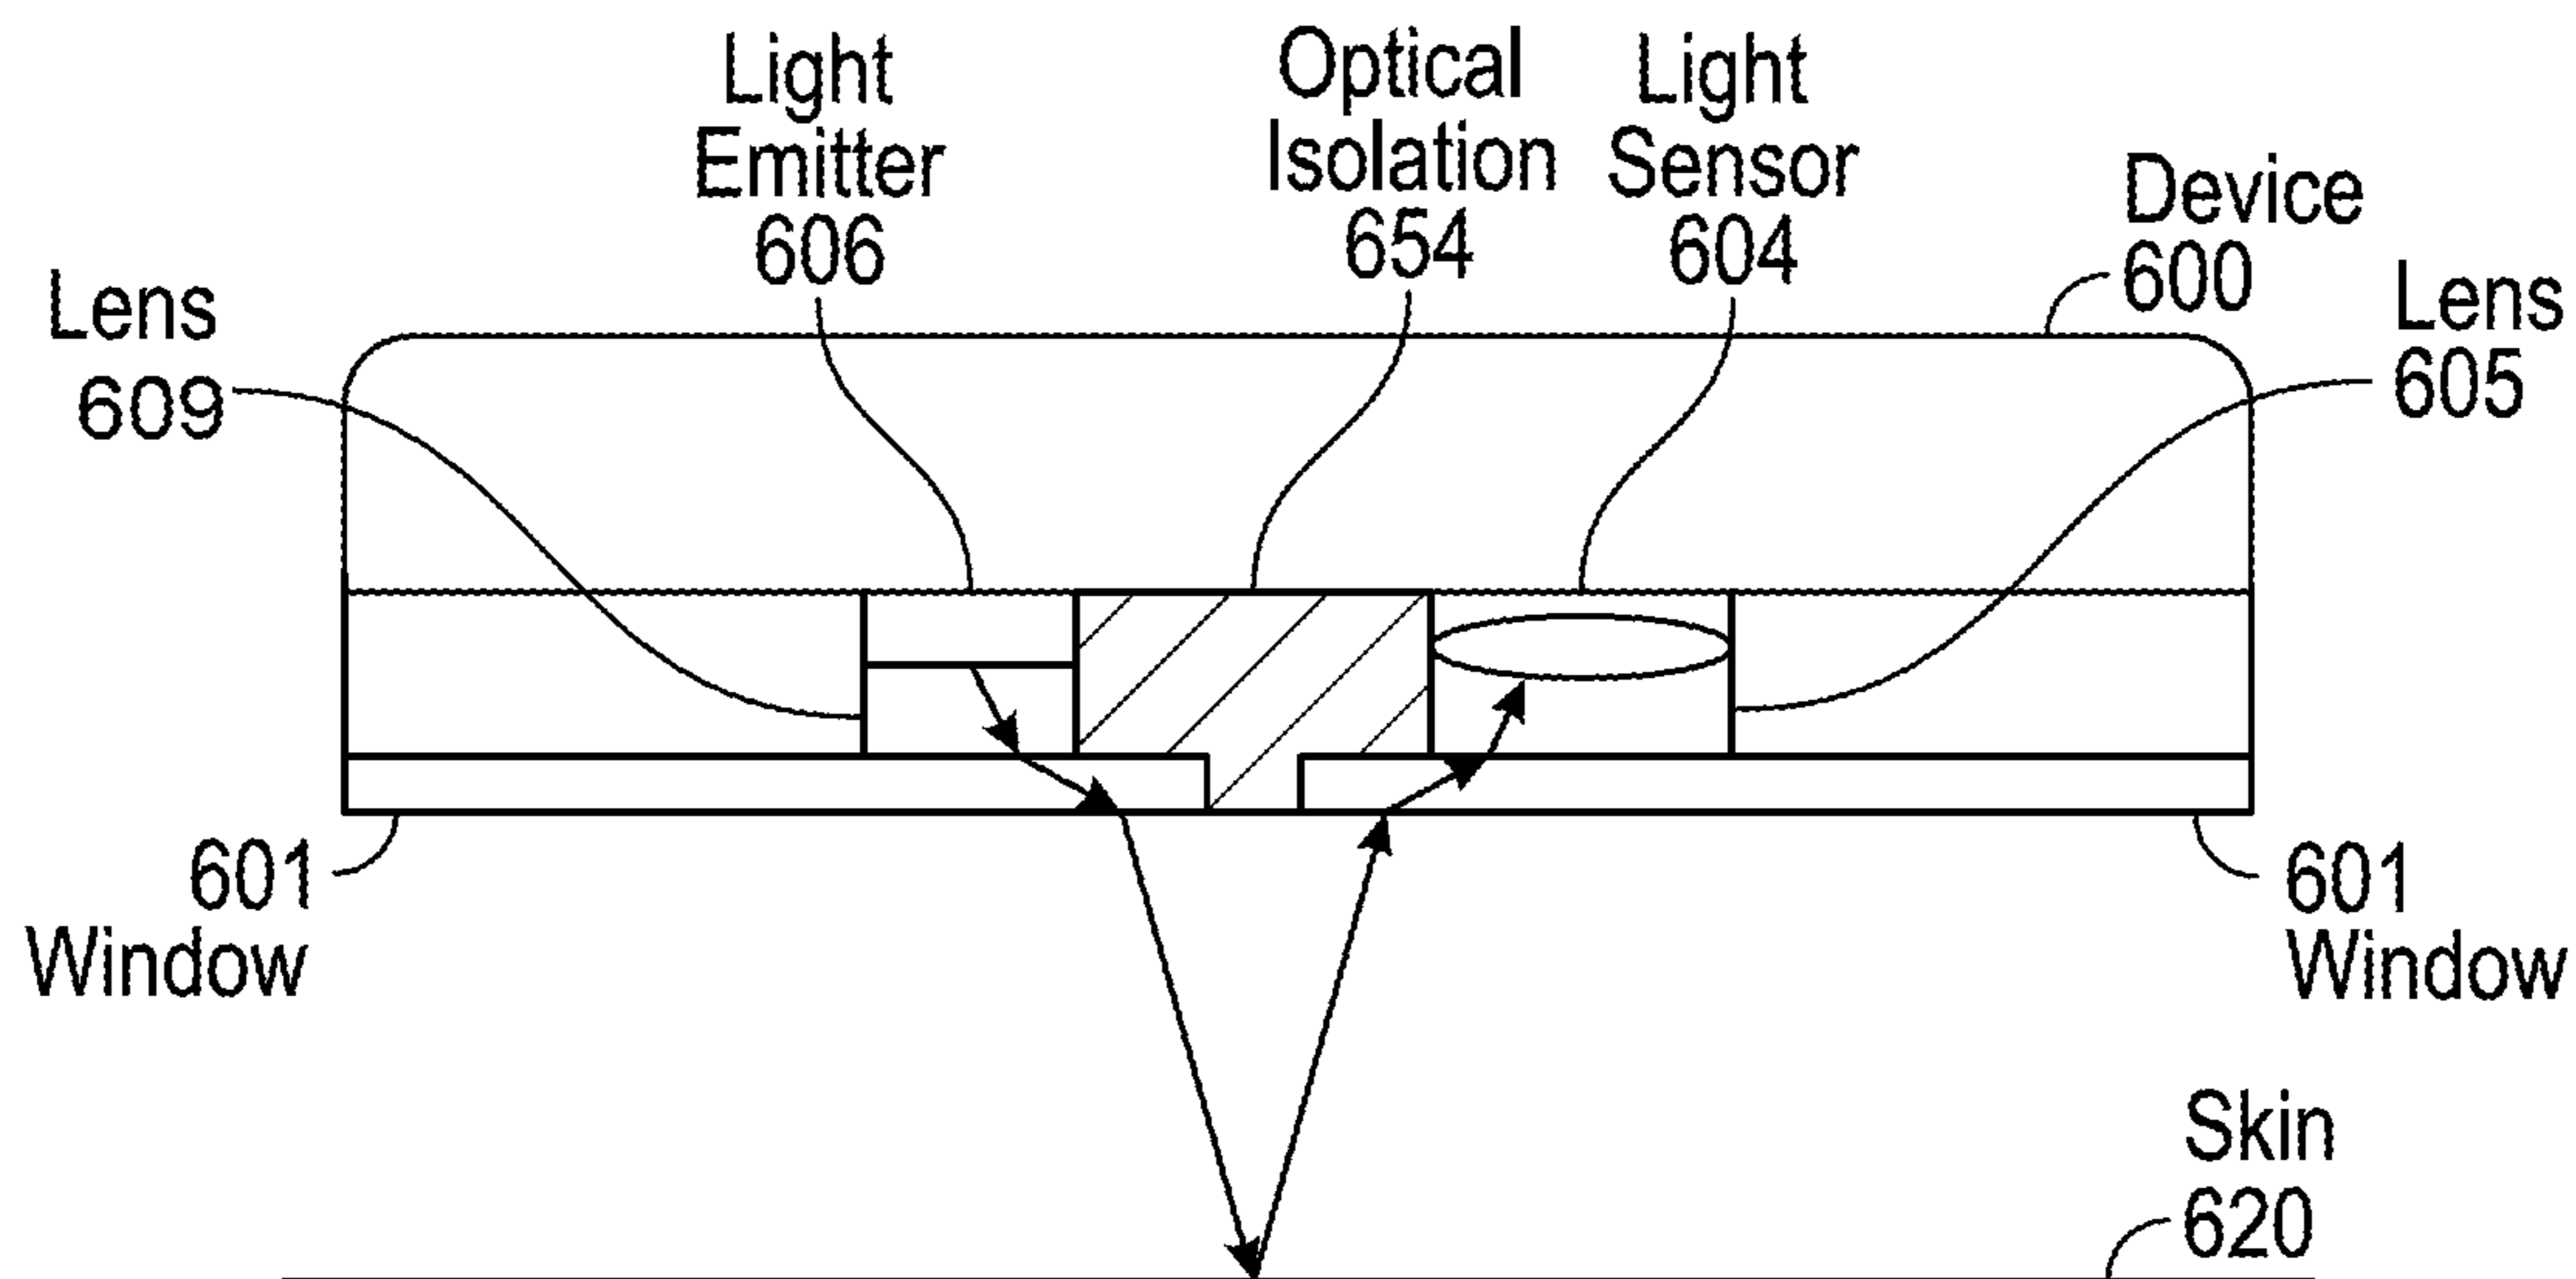


FIG. 6E

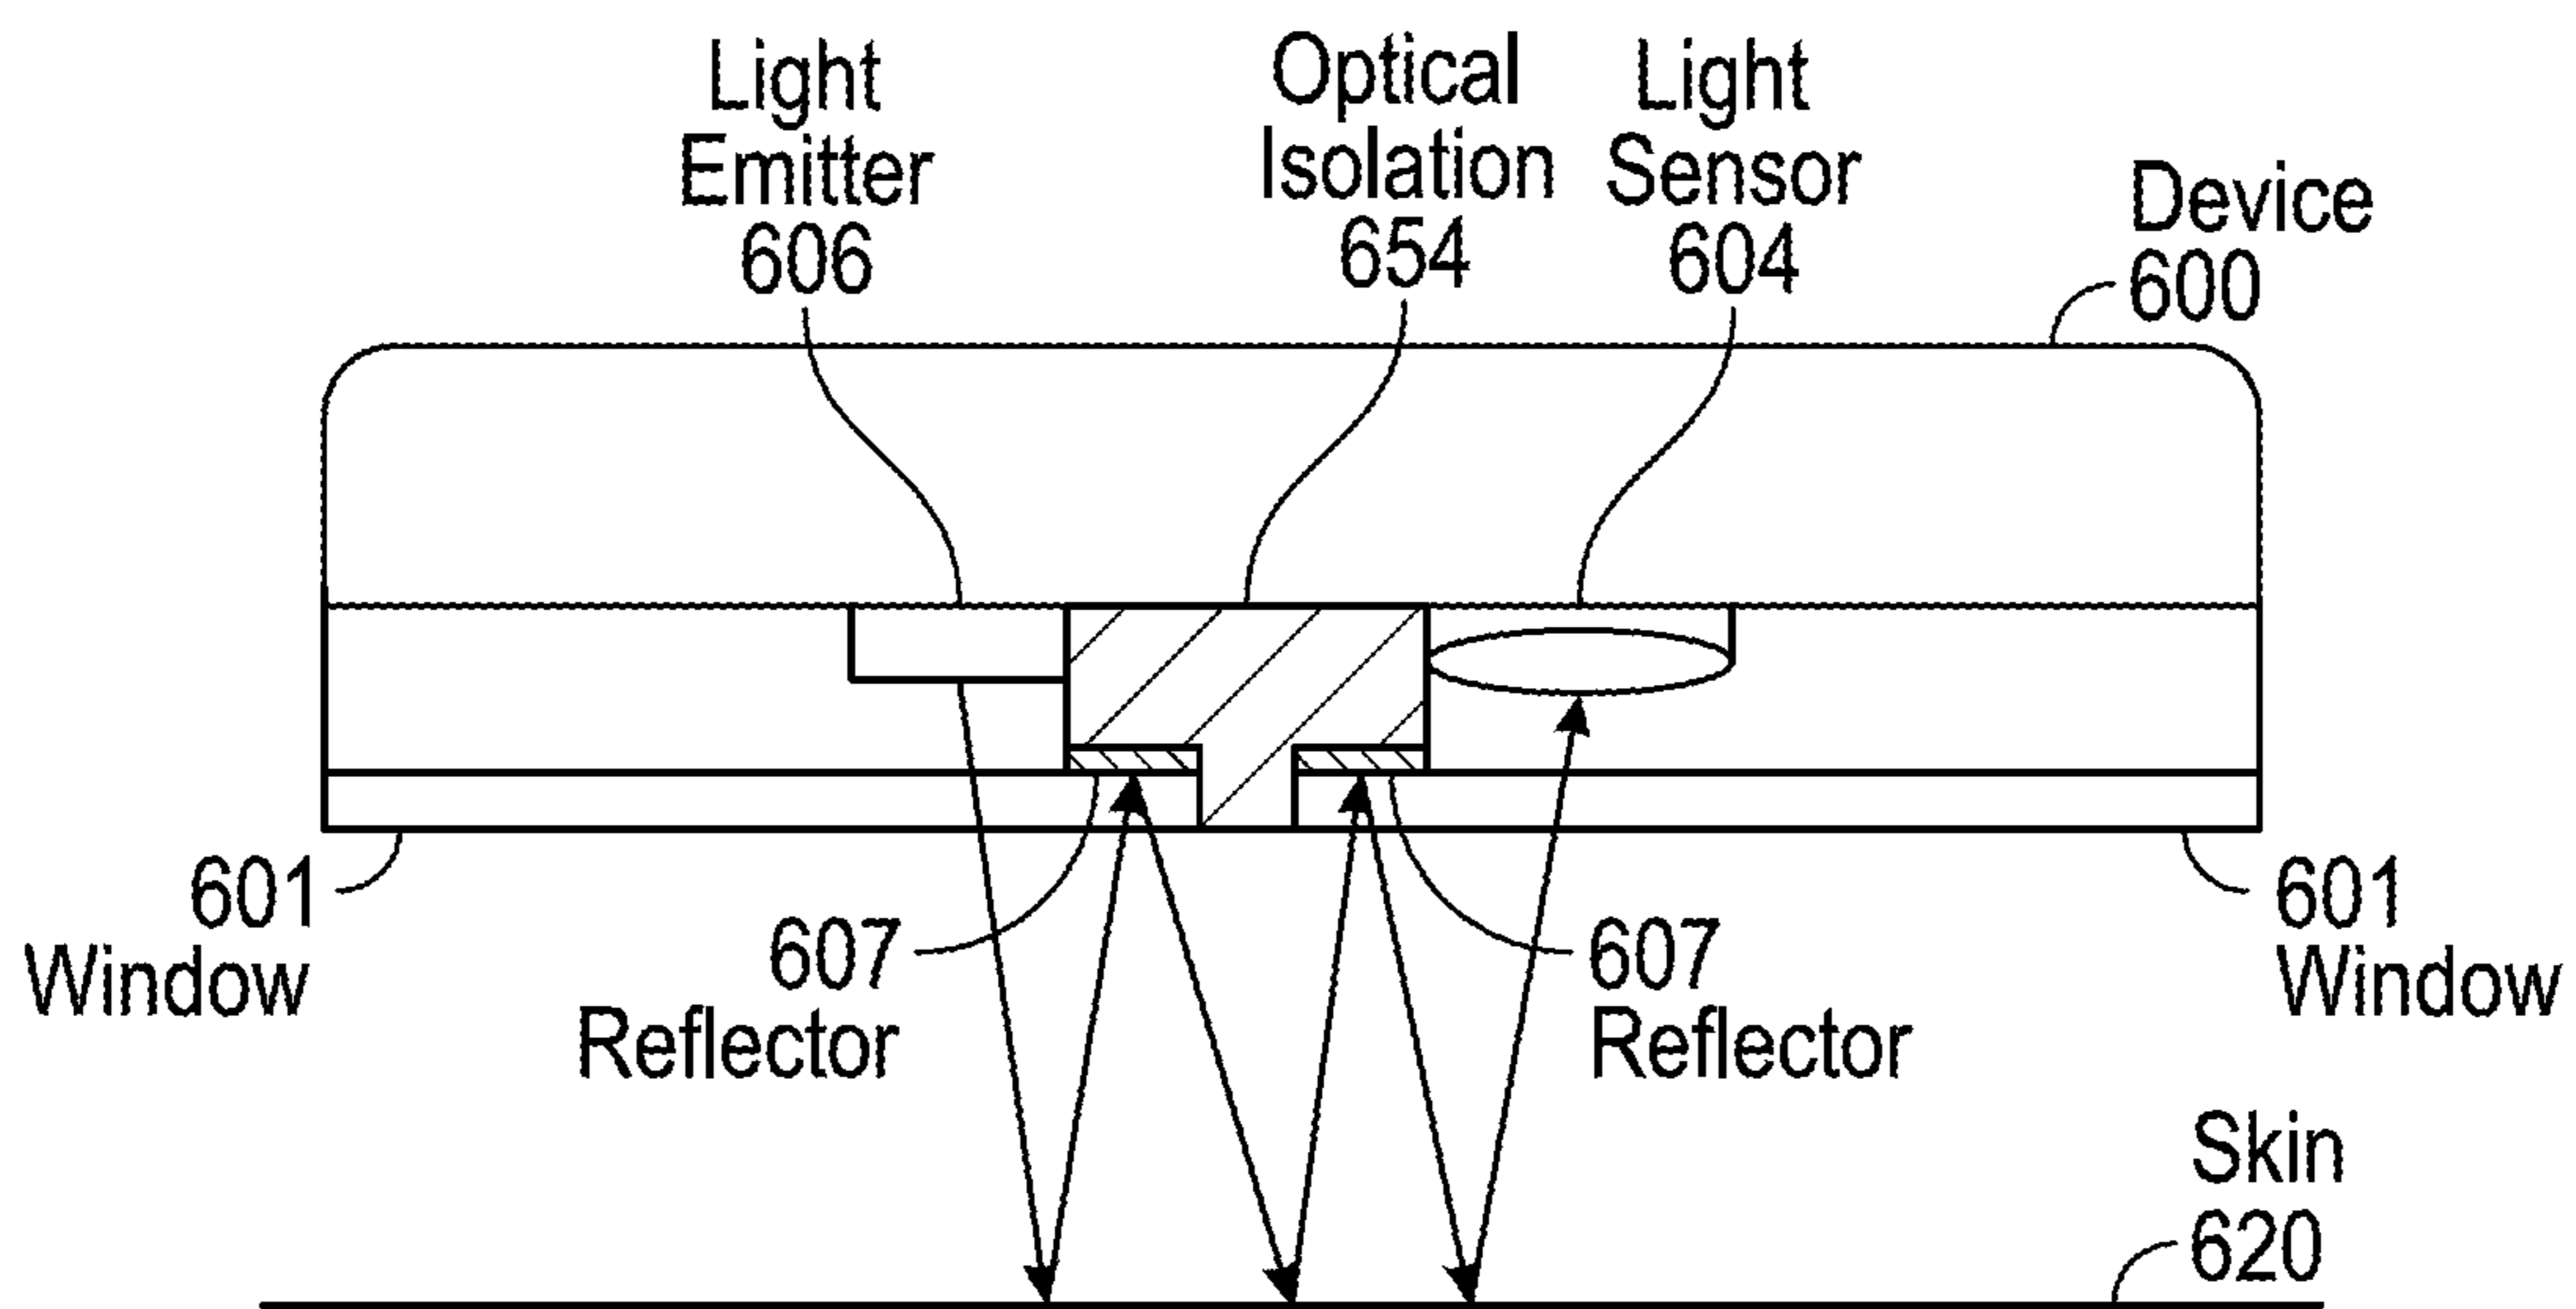


FIG. 6F

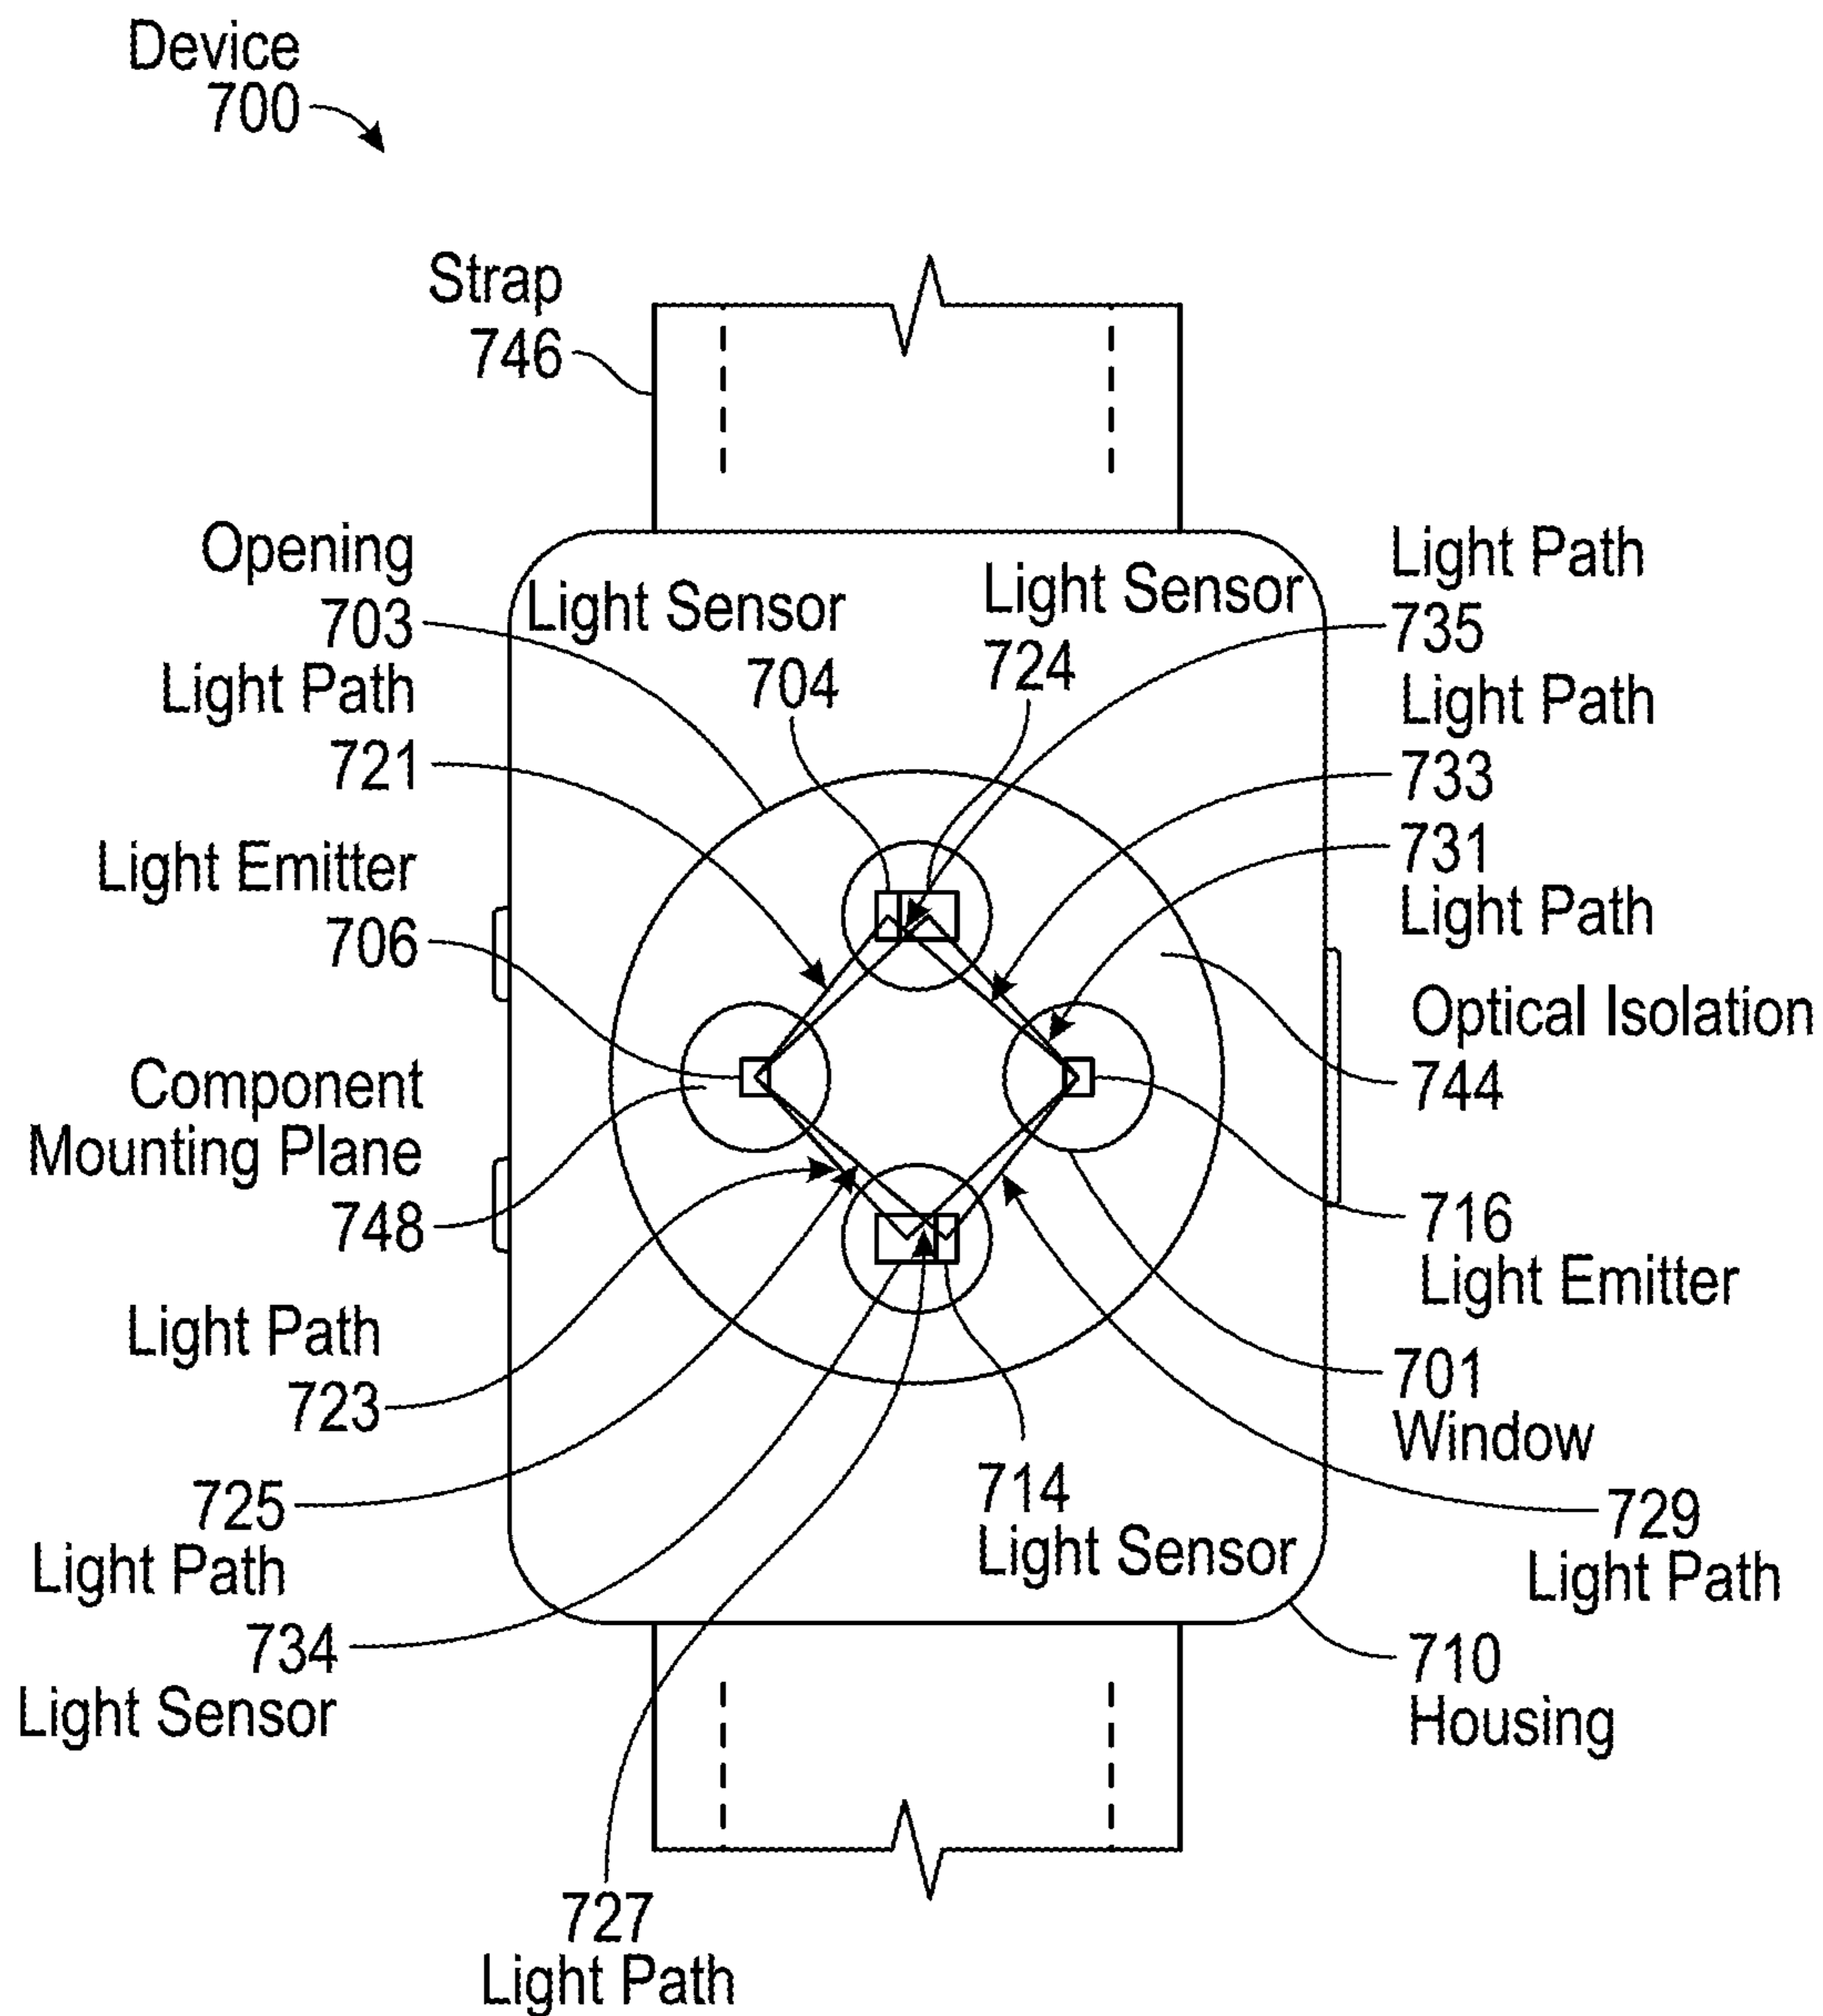


FIG. 7A

Light Path	Light Emitter	Light Sensor	Separation Distance
721	706	704	d1
723	706	734	d3
725	706	714	d4
727	716	734	d2
729	716	714	d1
731	716	724	d3
733	716	704	d4
735	706	724	d2

FIG. 7B

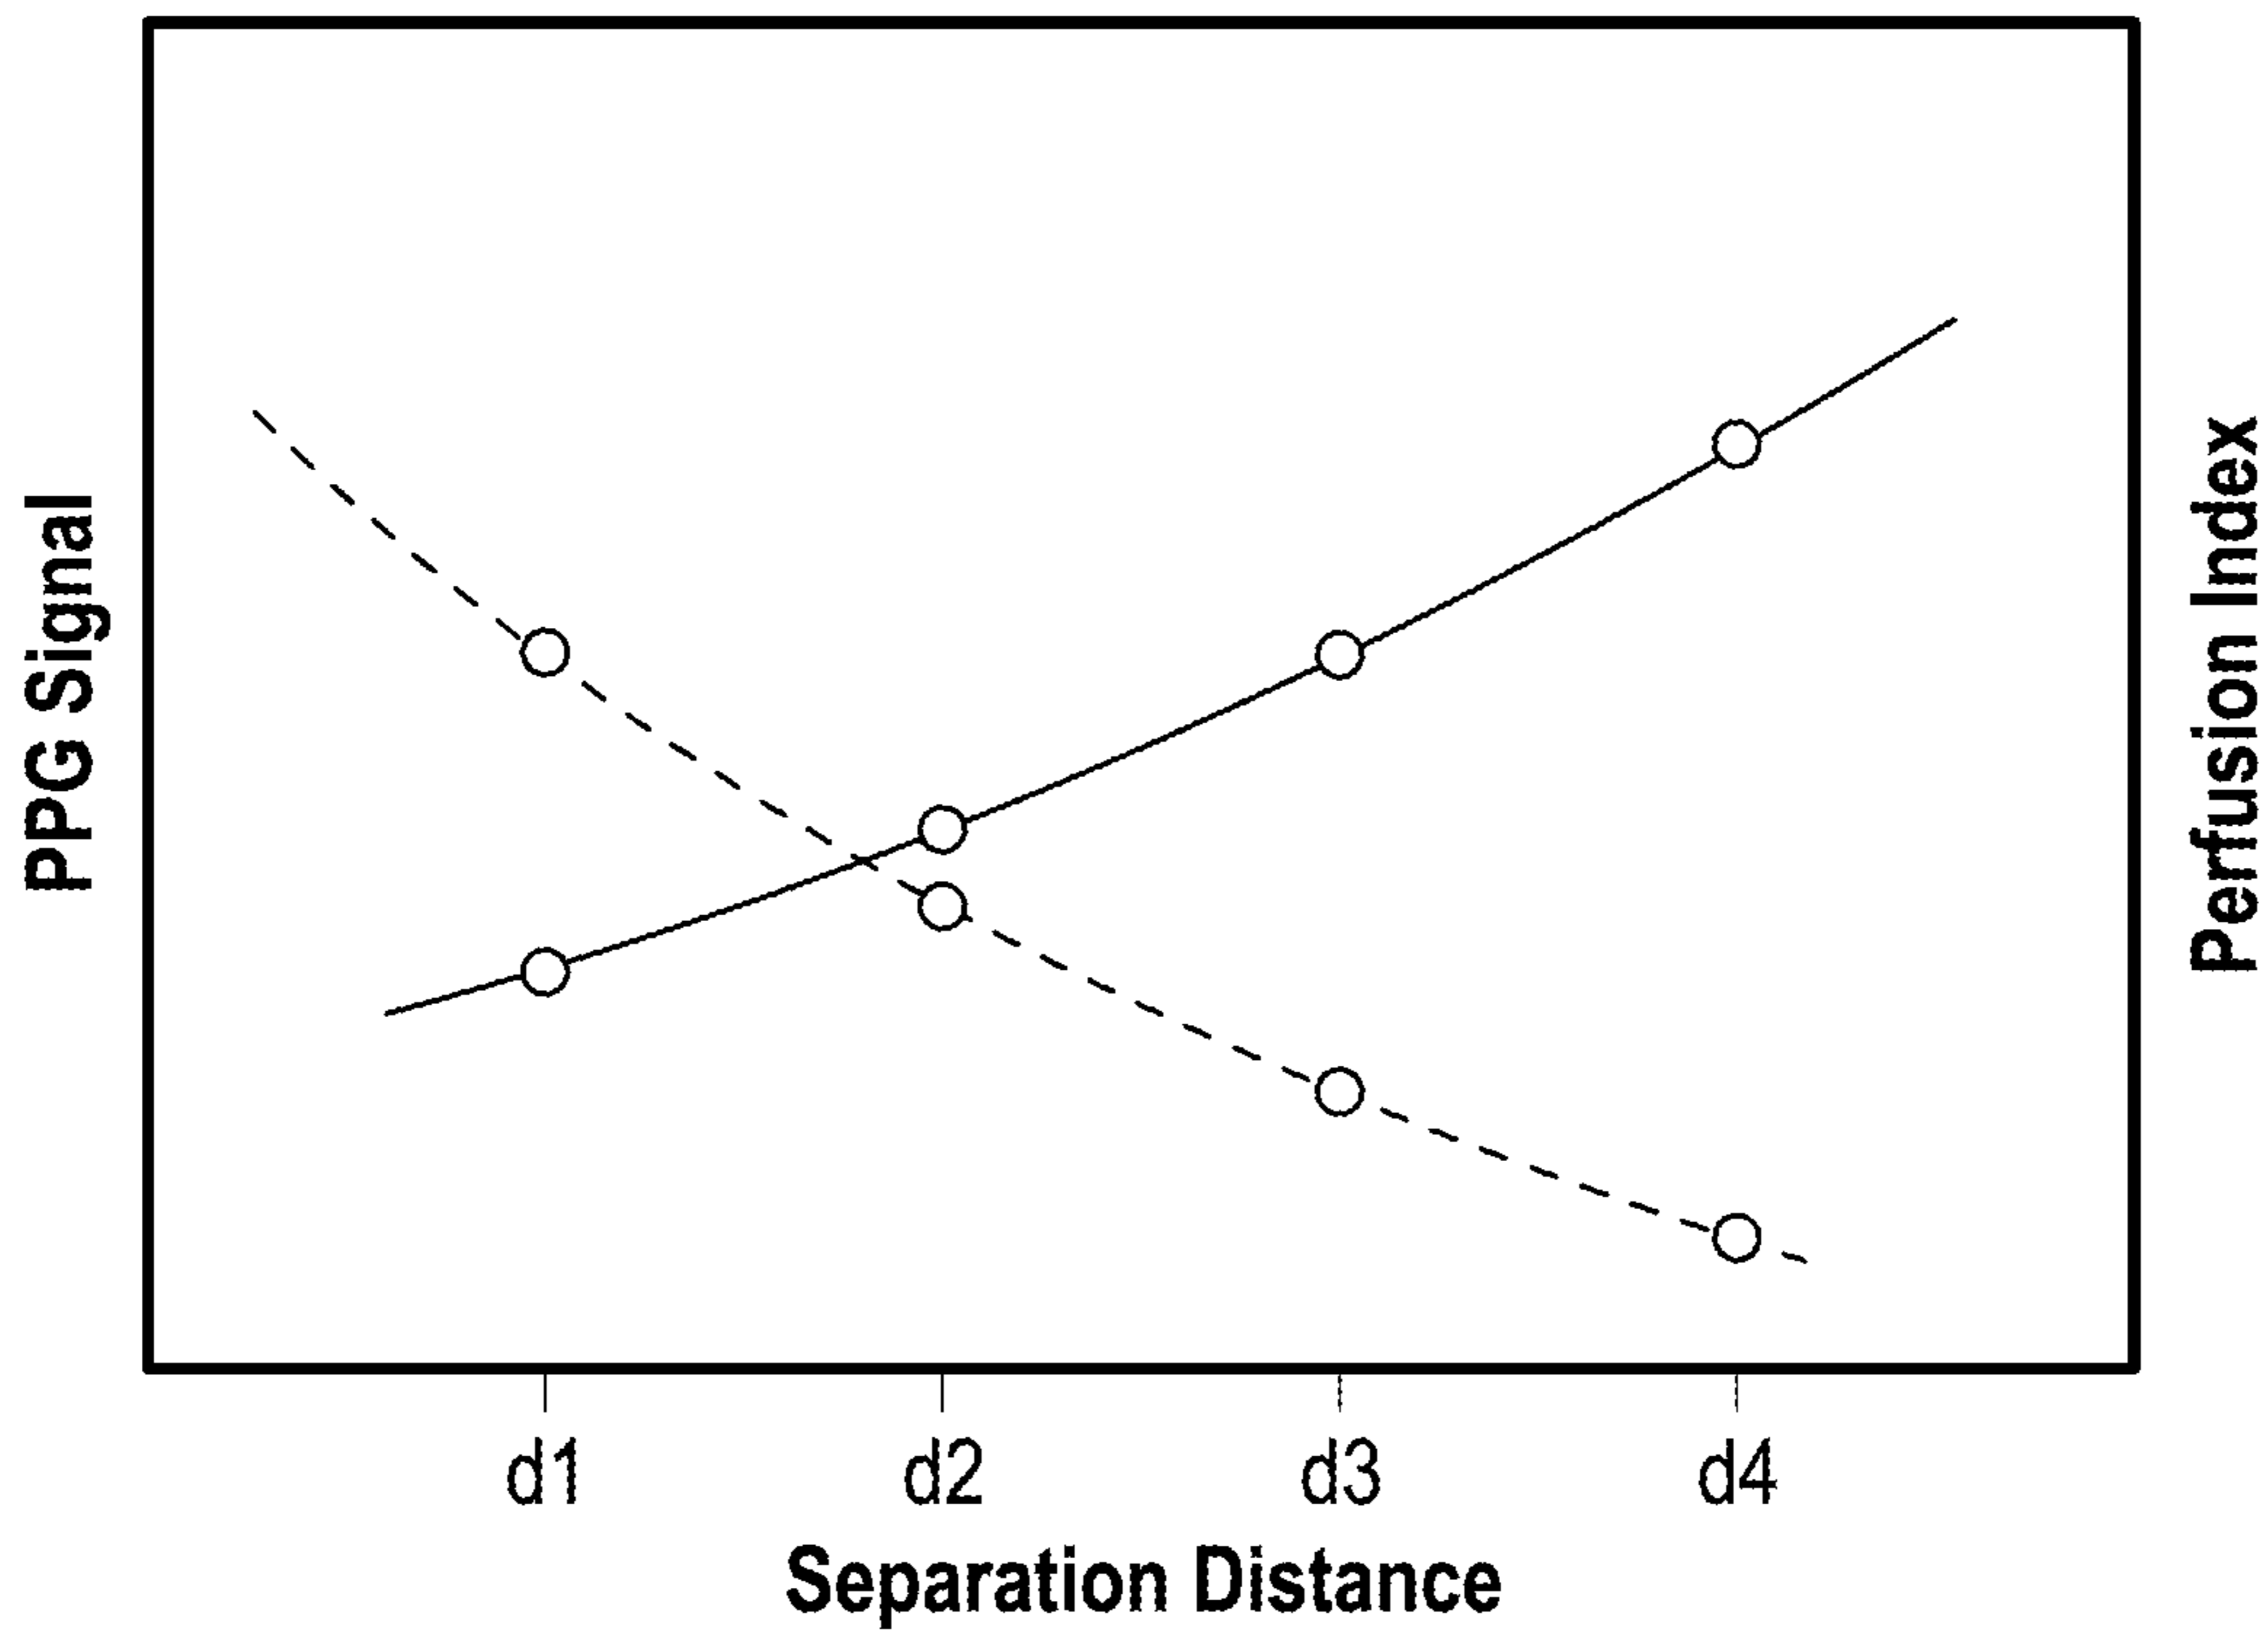
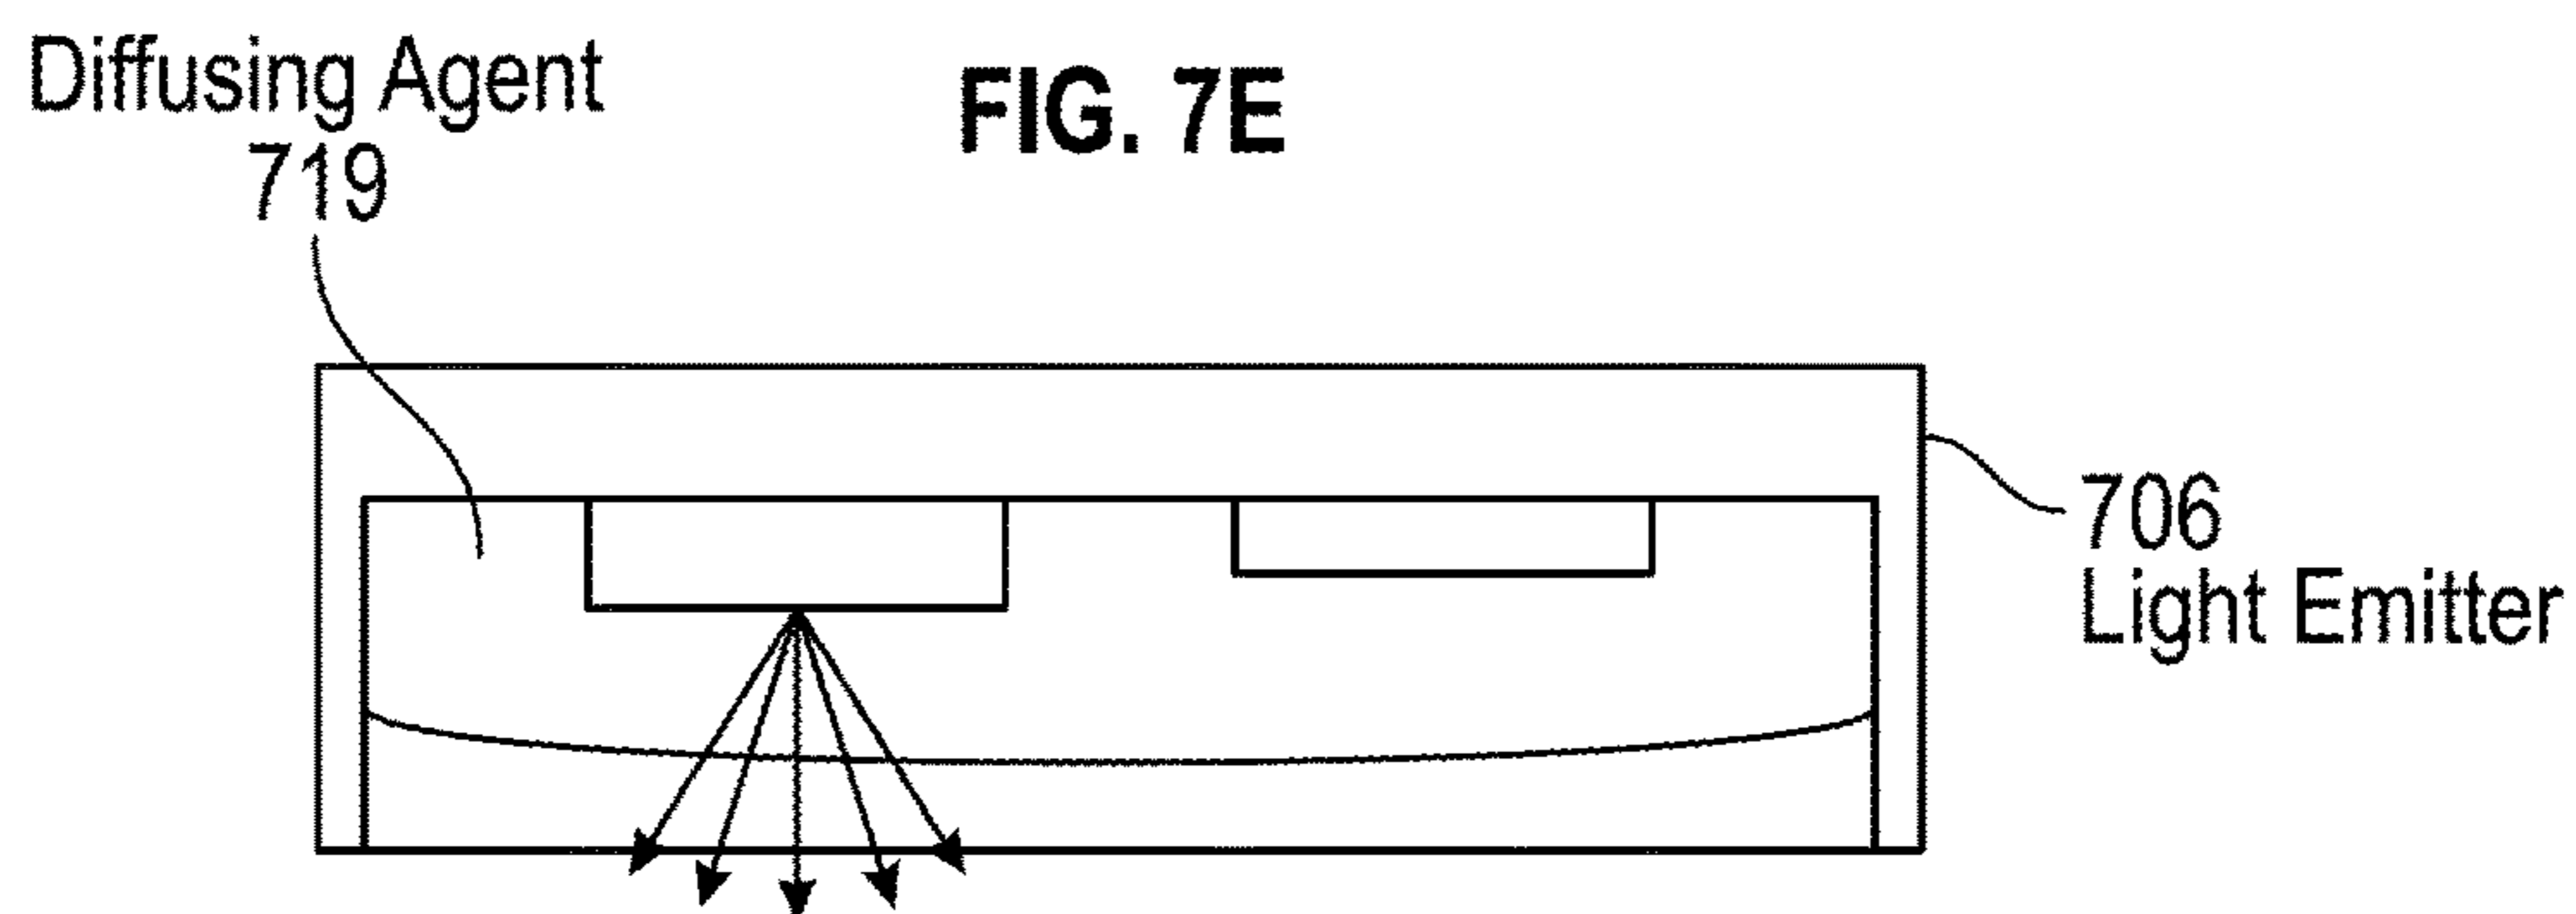
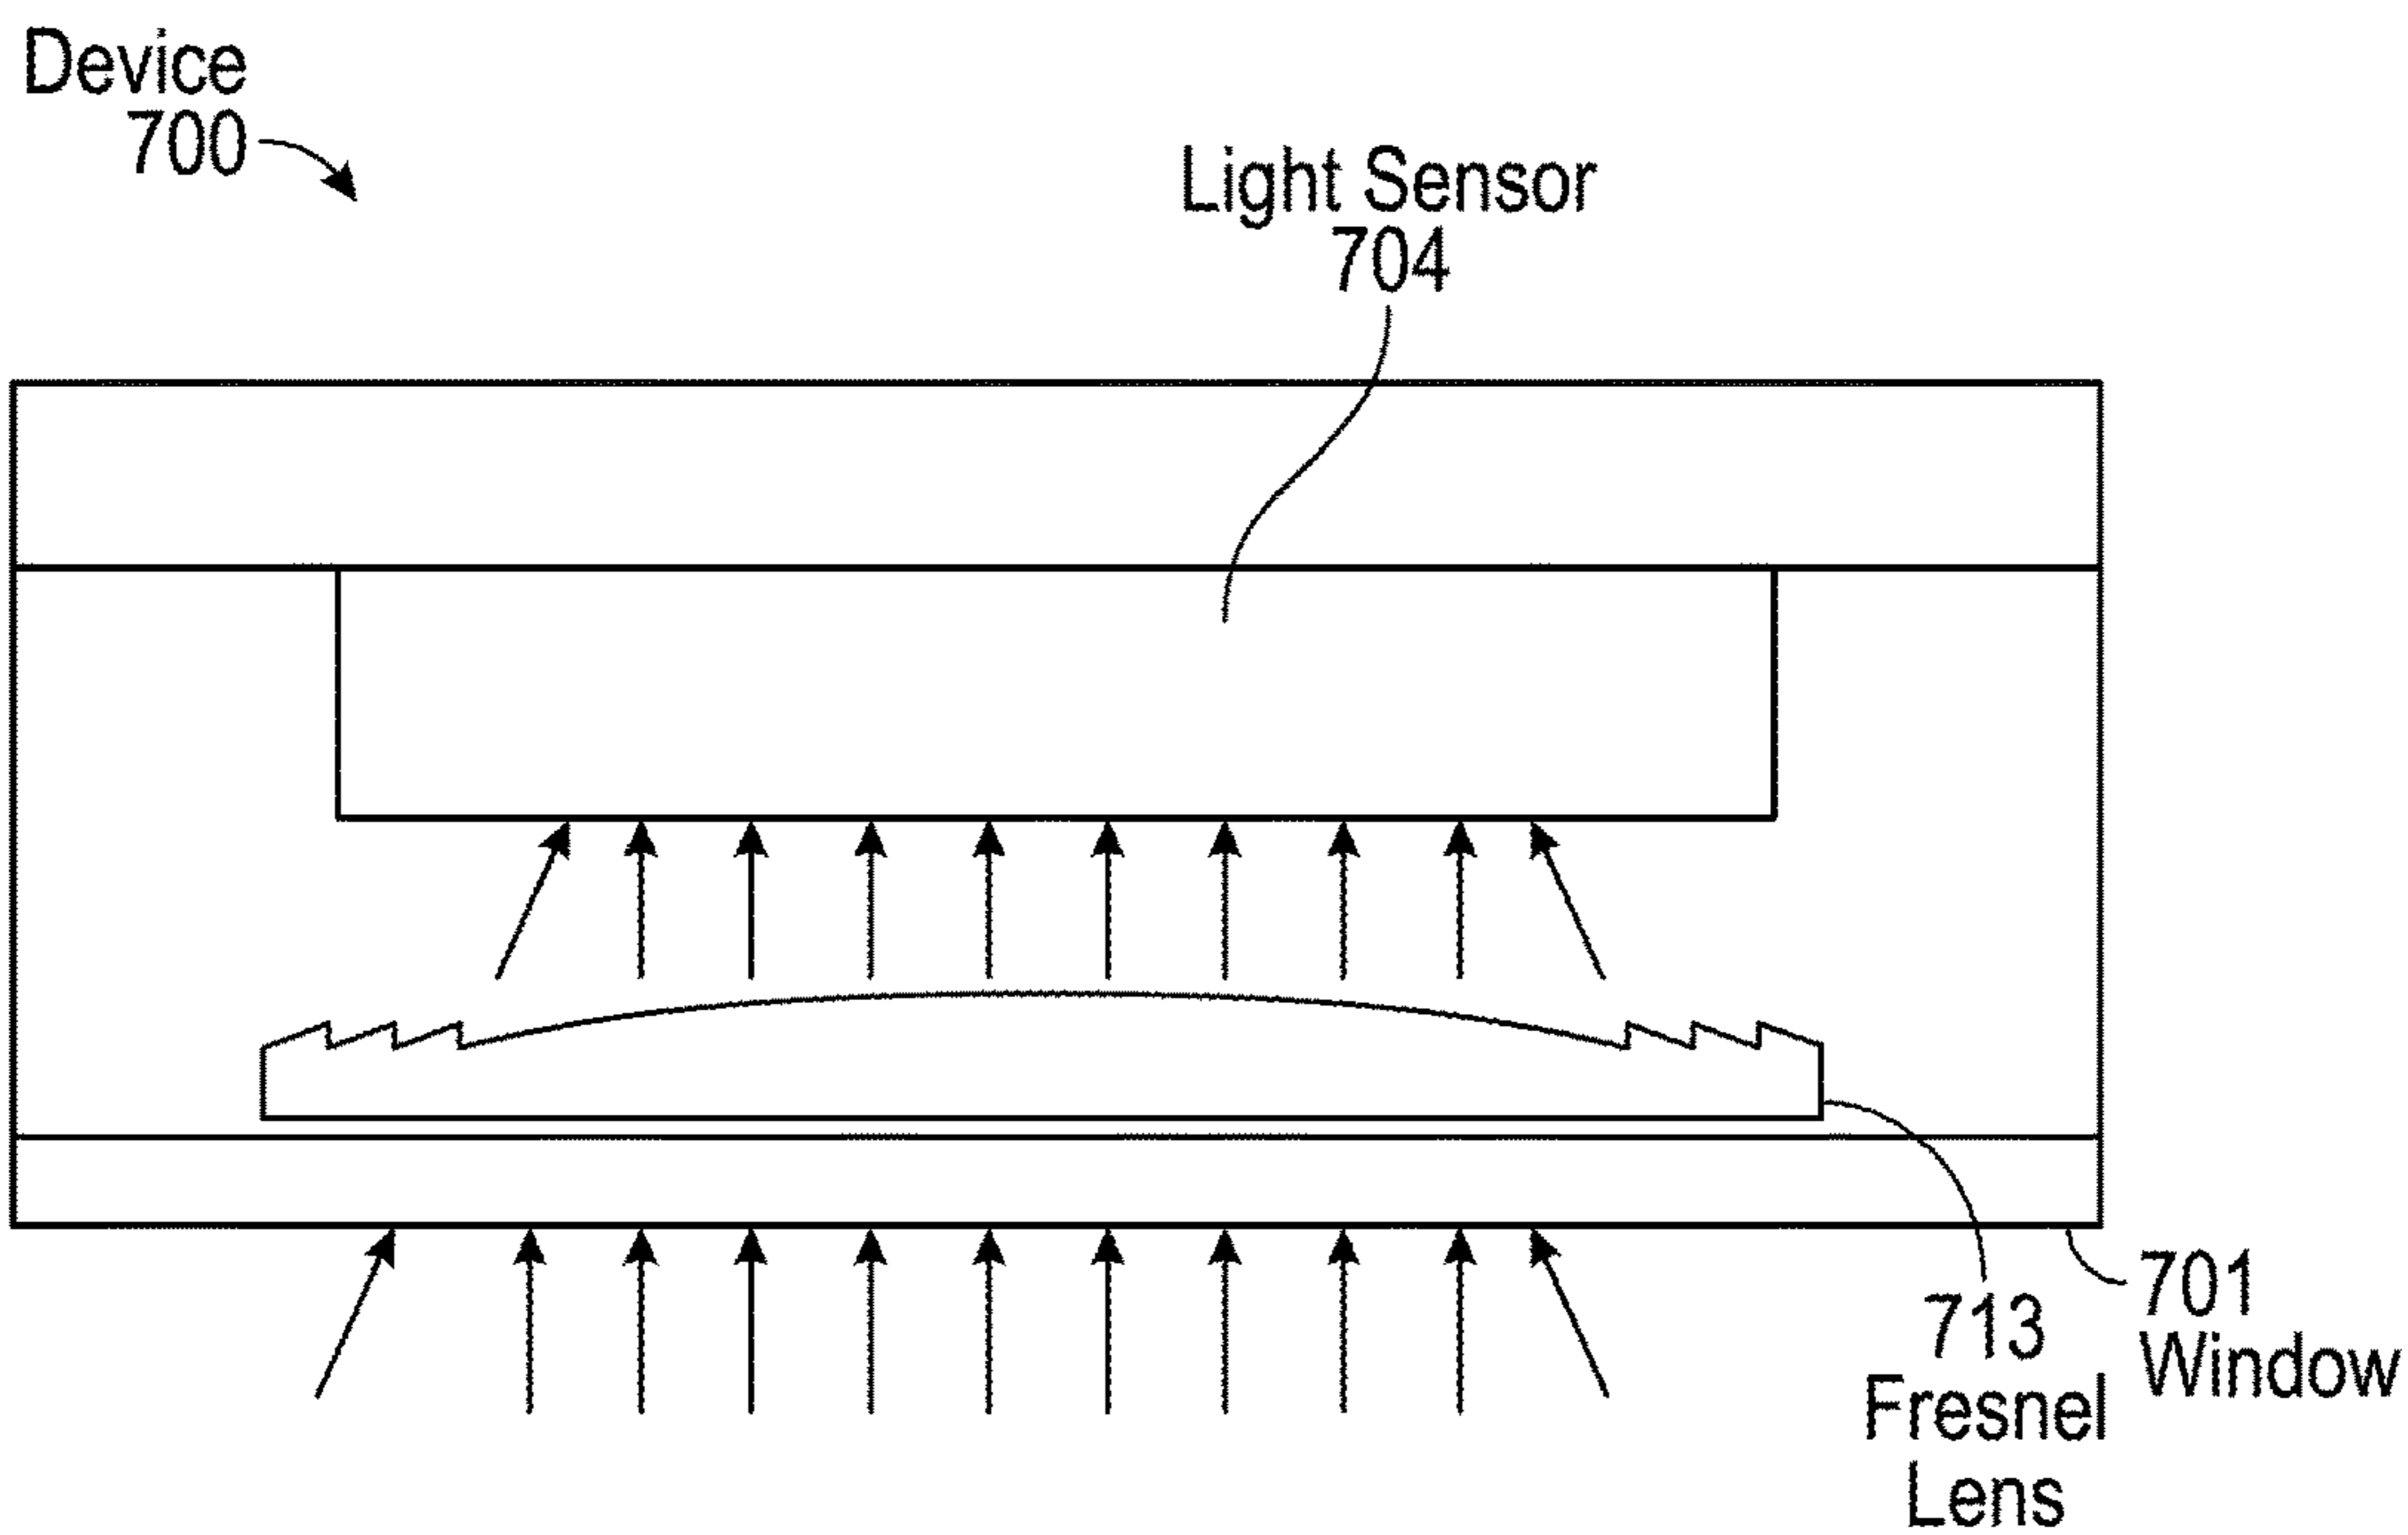
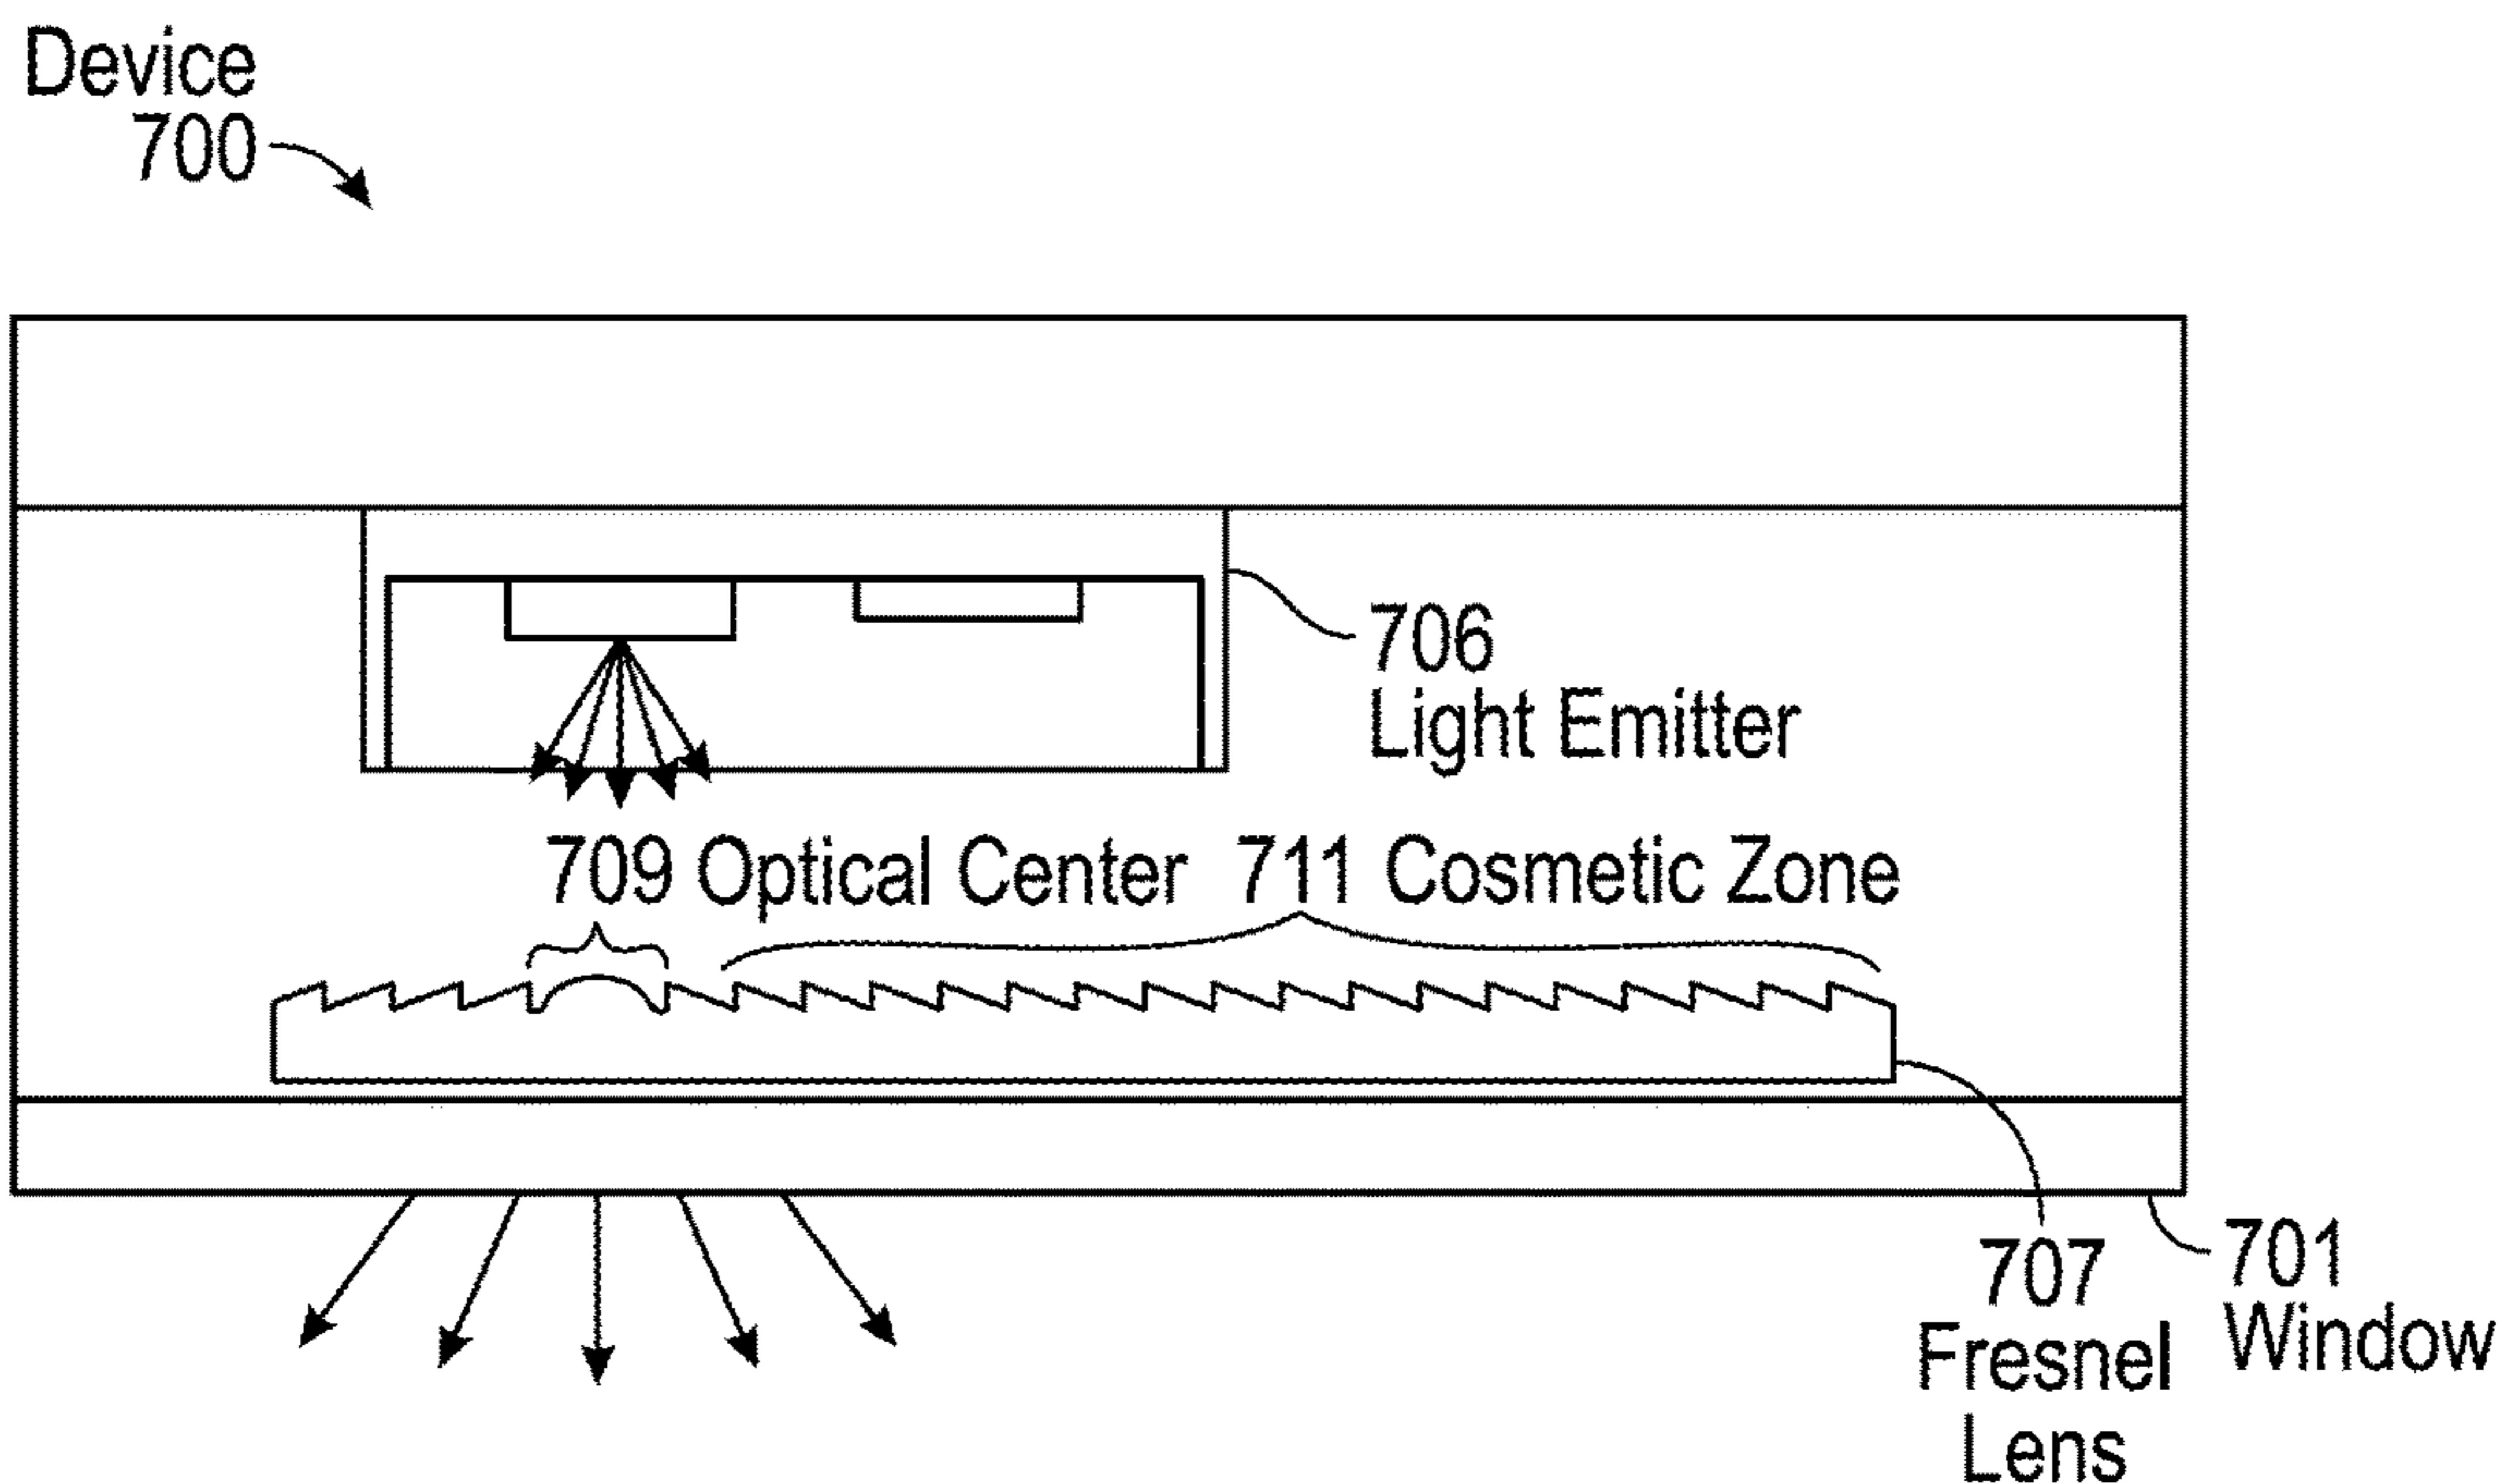


FIG. 7C



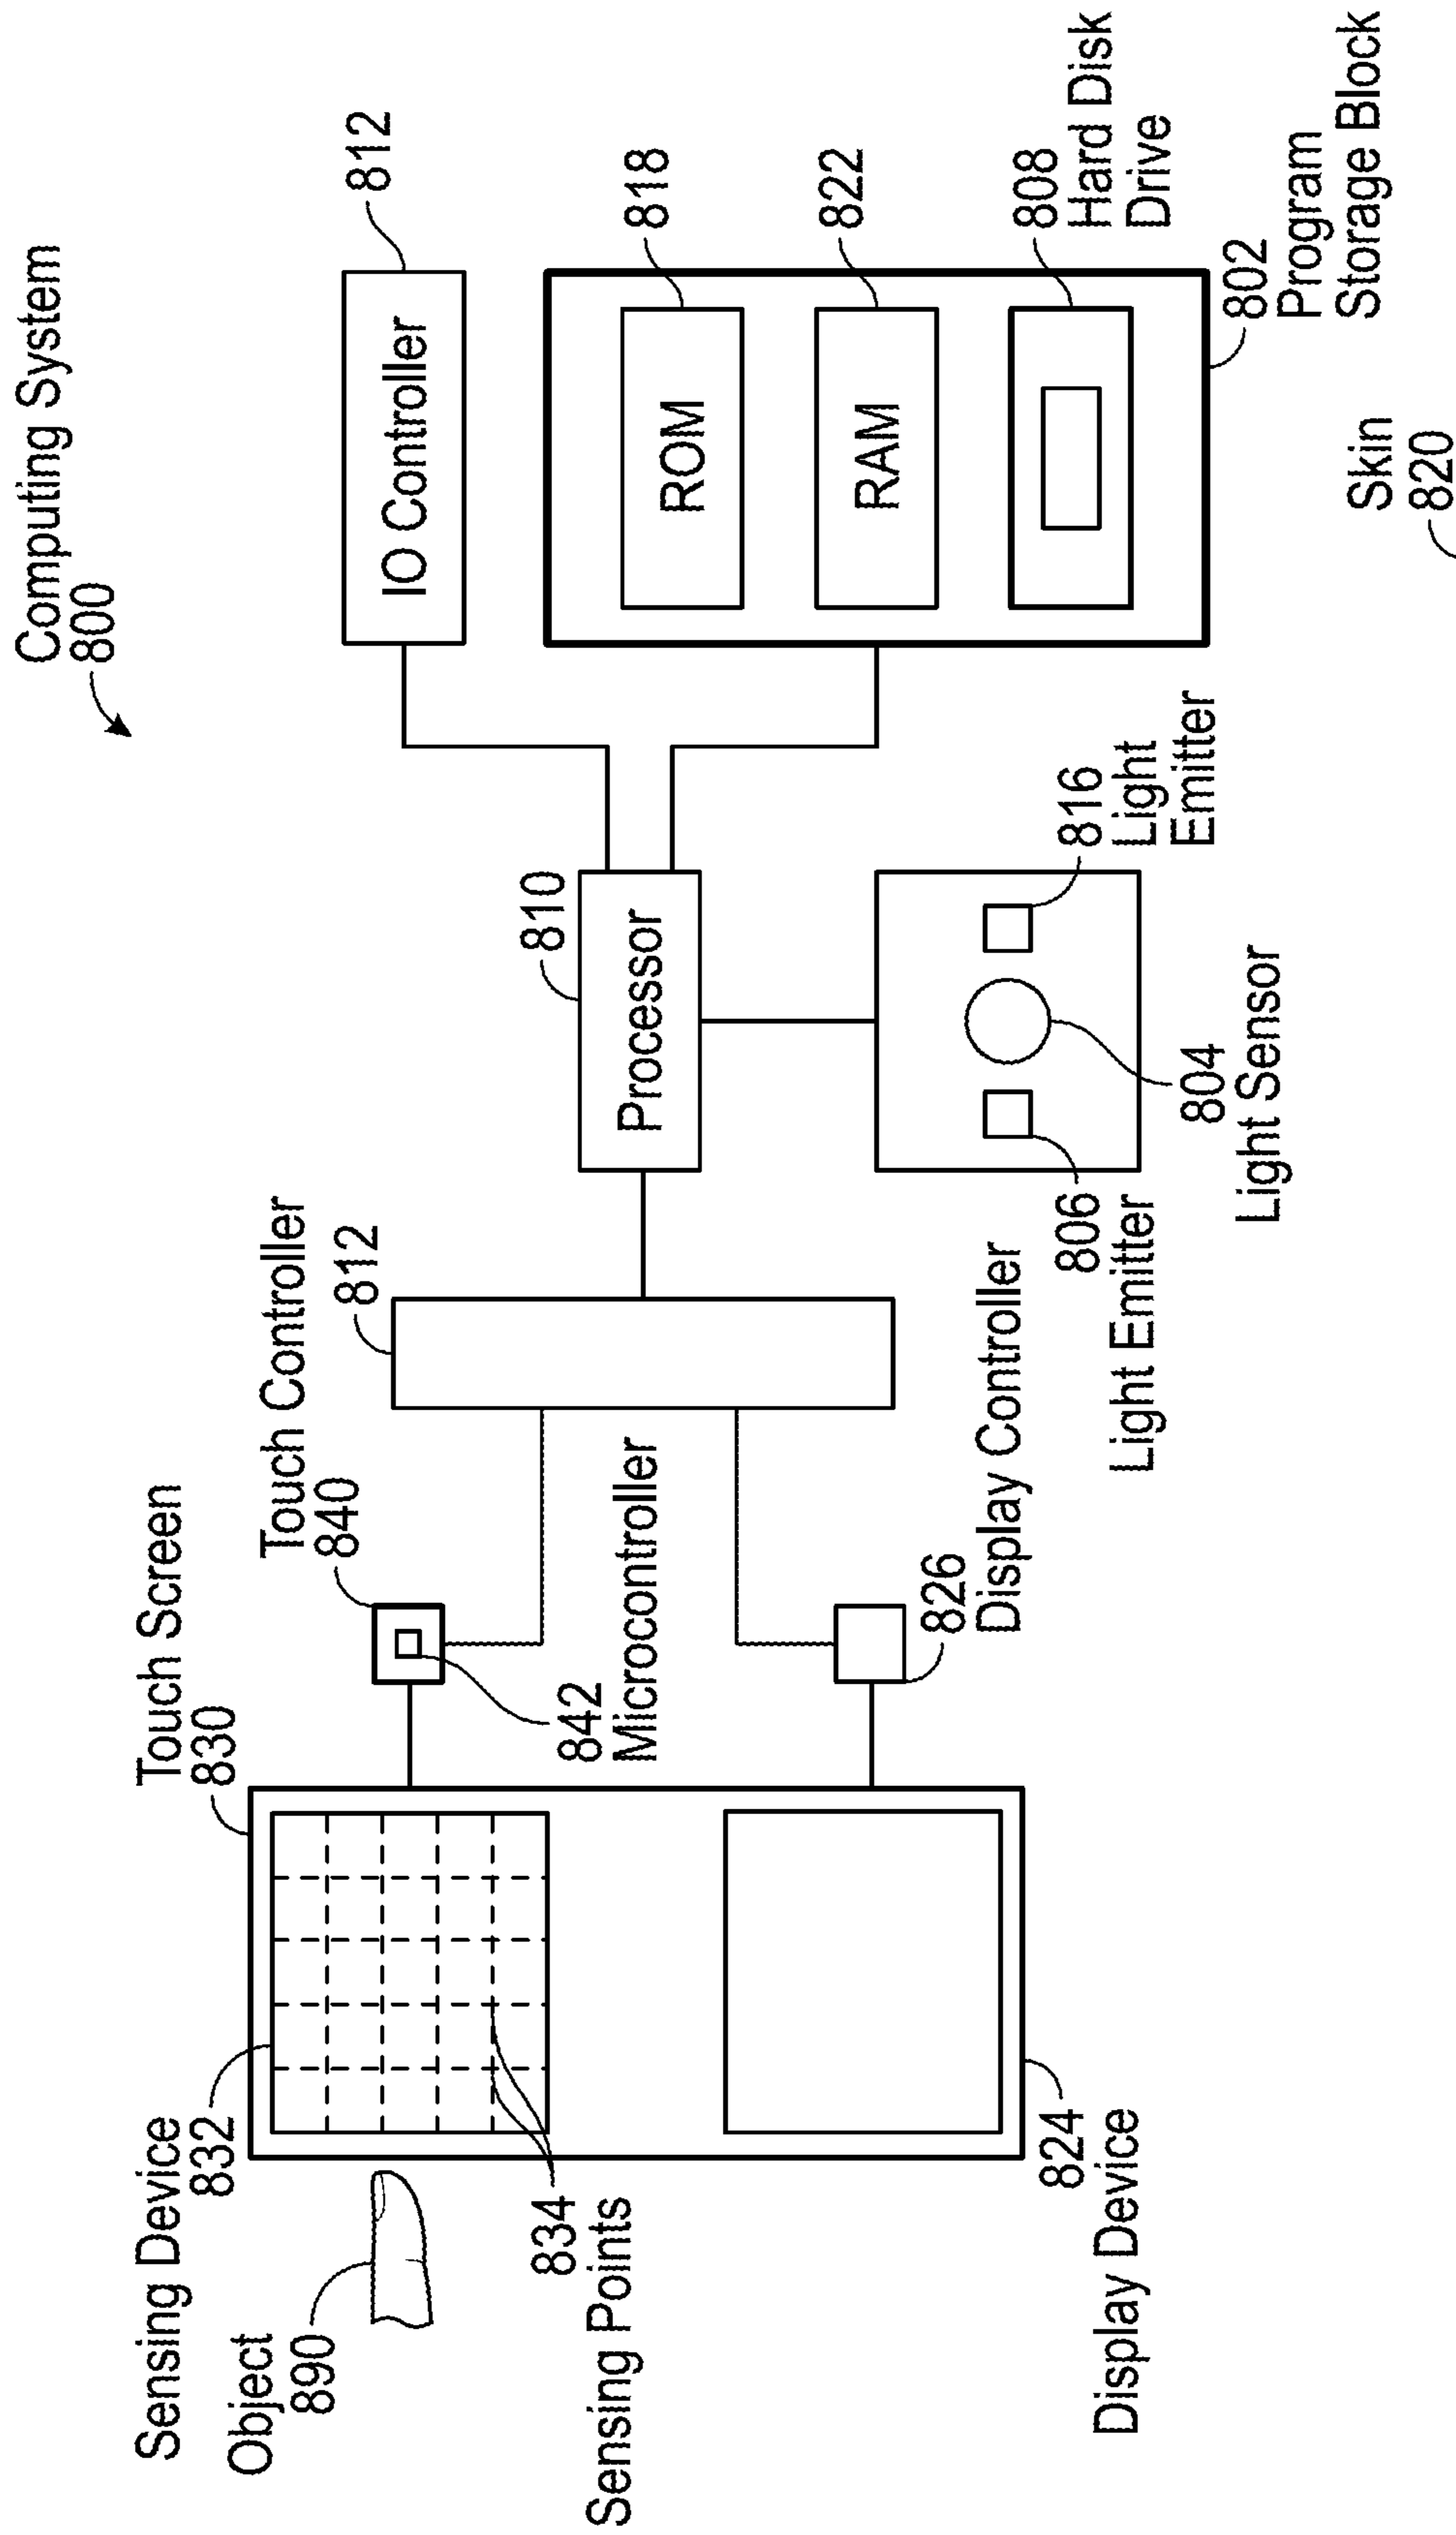


FIG. 8

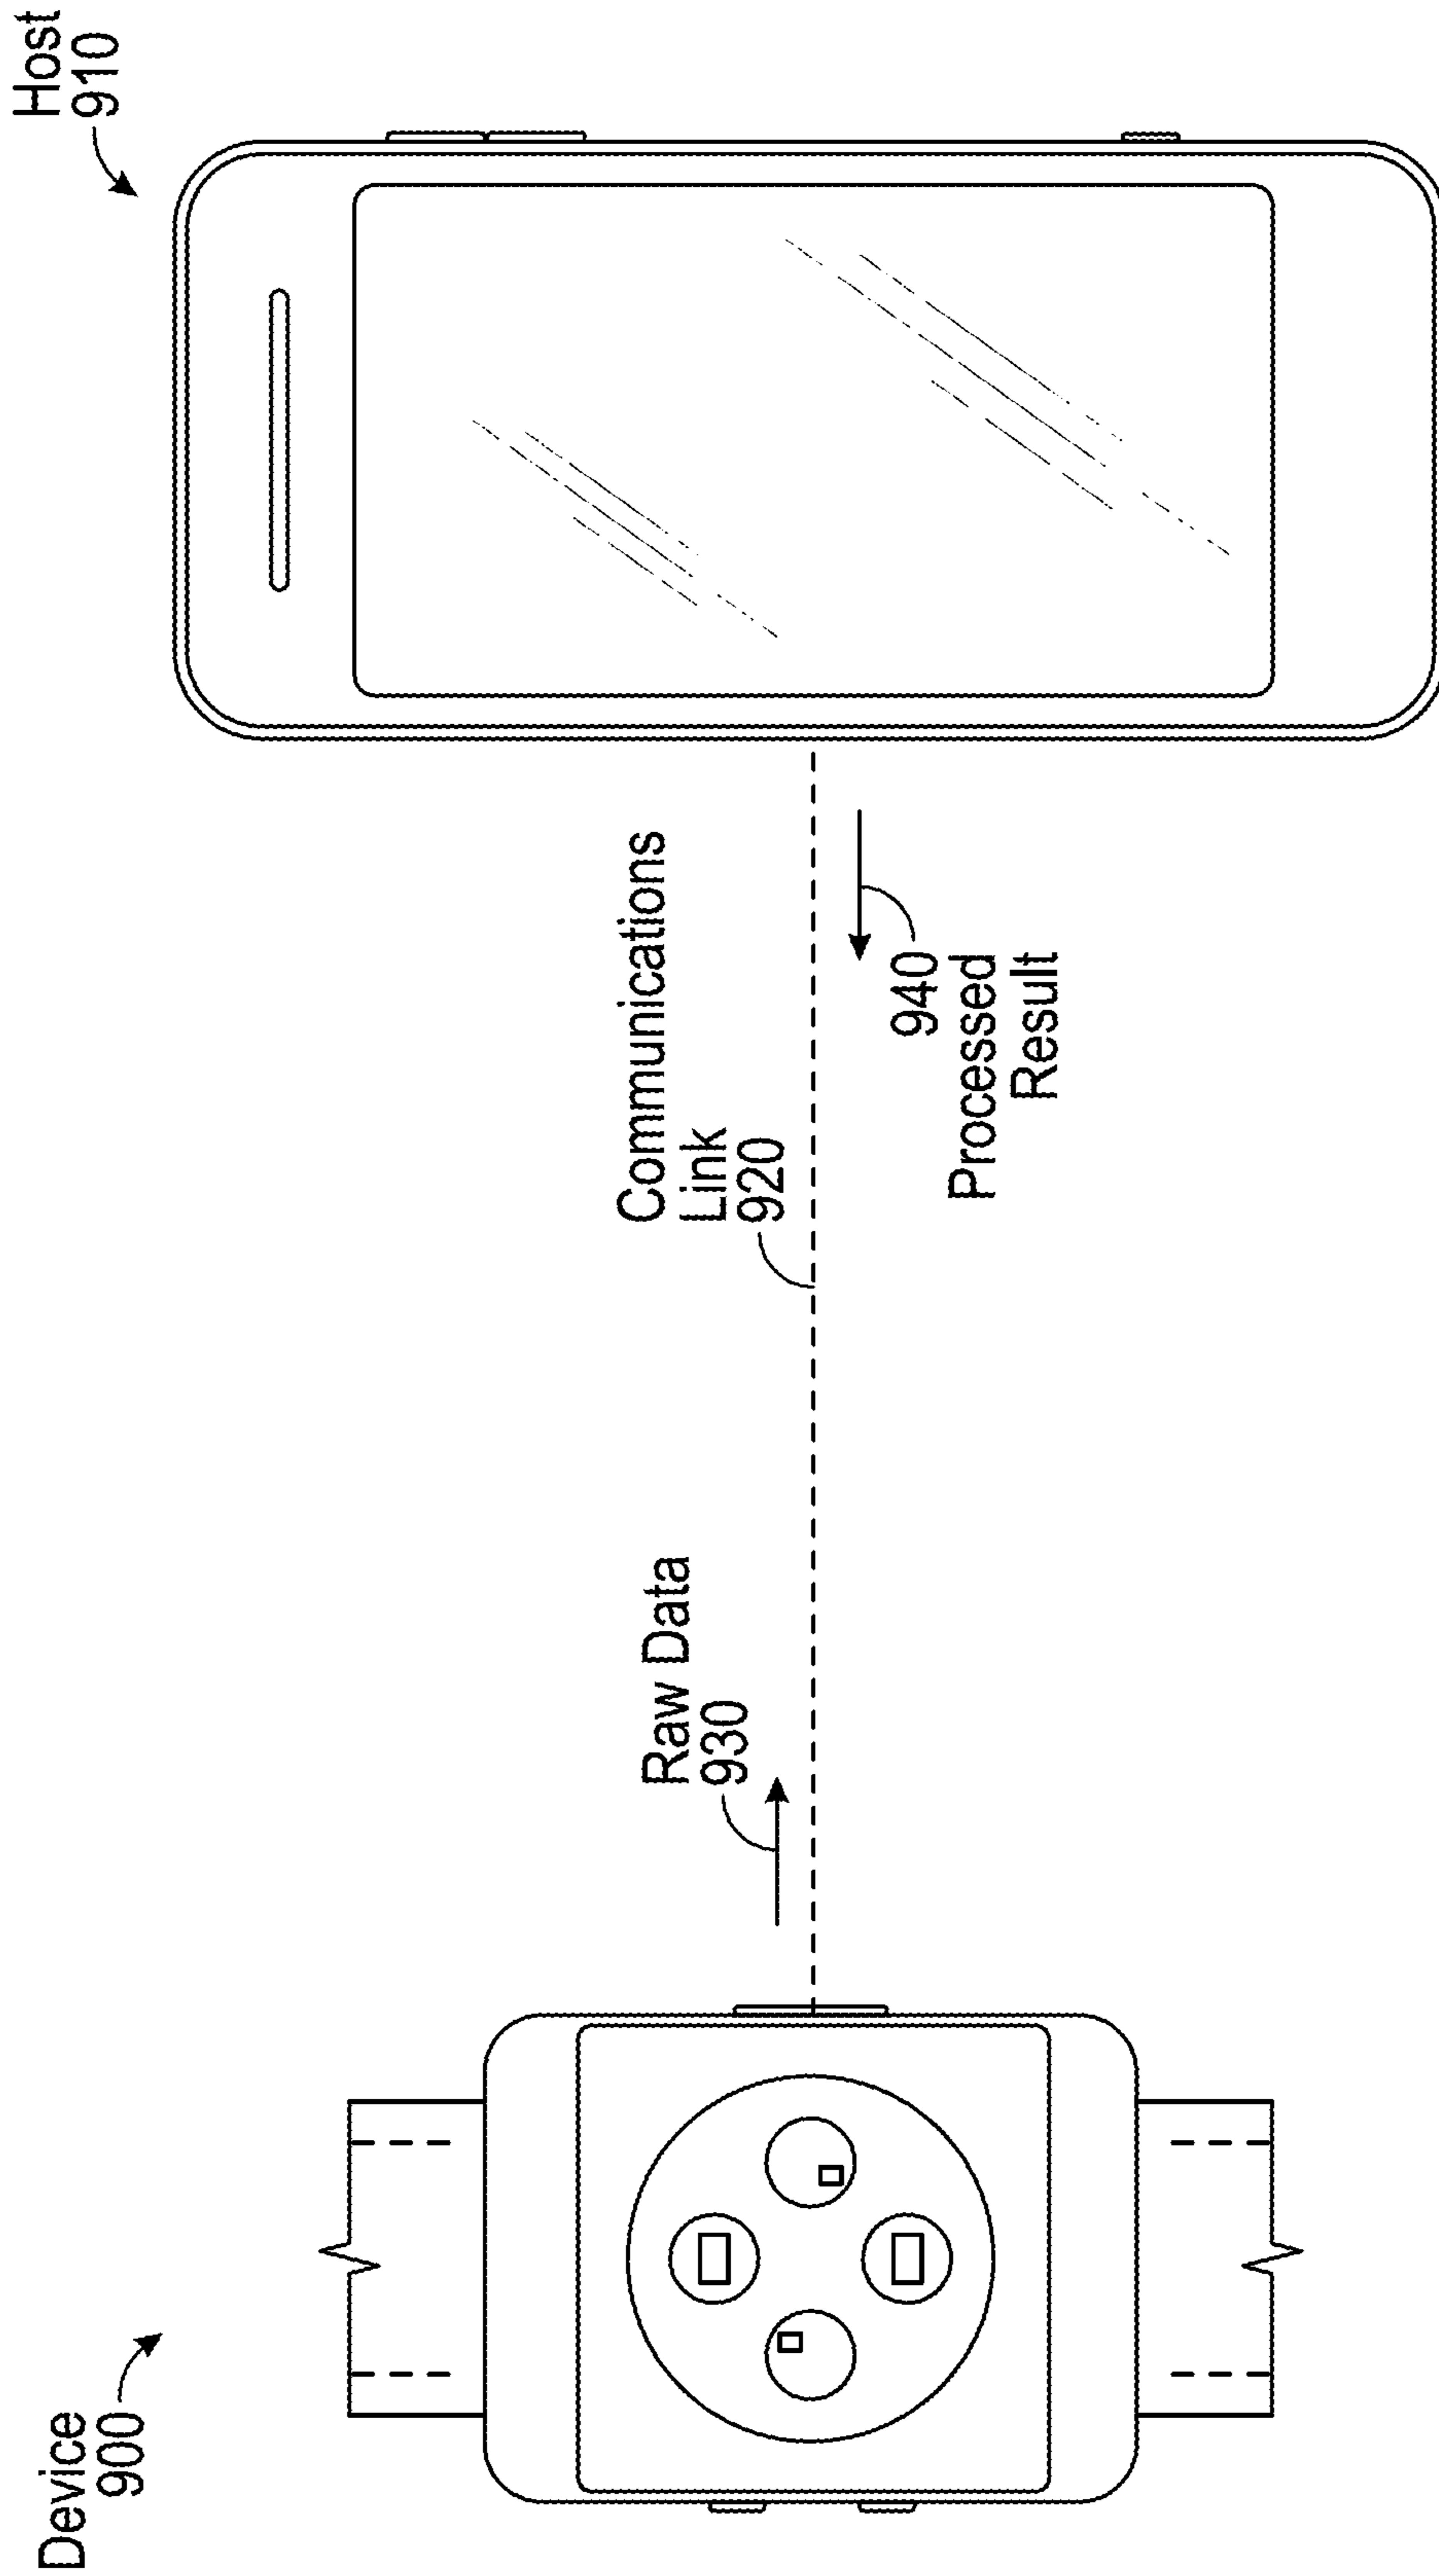


FIG. 9



**MULTIPLE LIGHT PATHS ARCHITECTURE  
AND OBSCURATION METHODS FOR  
SIGNAL AND PERFUSION INDEX  
OPTIMIZATION**

CROSS REFERENCE TO RELATED  
APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 16/144,958, filed Sep. 27, 2018, which is a continuation of U.S. patent application Ser. No. 14/569,235, filed Dec. 12, 2014, now U.S. Pat. No. 10,215,698, which claims the benefit under 35 U.S.C. § 119(e) of U.S. Patent Application No. 62/044,515, filed Sep. 2, 2014, the contents of which are incorporated herein by reference in their entirety for all purposes.

FIELD

This relates generally to a device that measures a photoplethysmographic (PPG) signal, and, more particularly, to architectures for multiple light paths and obscuration methods for PPG signal and perfusion index optimization.

BACKGROUND

A photoplethysmographic (PPG) signal can be measured by PPG systems to derive corresponding physiological signals (e.g., pulse rate). In a basic form, PPG systems can employ a light source or light emitter that injects light into the user's tissue and a light detector to receive light that reflects and/or scatters and exits the tissue. The received light includes light with an amplitude that is modulated as a result of pulsatile blood flow (i.e., "signal") and parasitic, non-signal light with an amplitude that can be modulated (i.e., "noise" or "artifacts") and/or unmodulated (i.e., DC). Noise can be introduced by, for example tilt and/or pull of the device relative to the user's tissue, hair, and/or motion.

For a given light emitter and light detector, the PPG pulsatile signal (i.e., detected light modulated by pulsatile blood flow) can decrease as the separation distance between the light emitter and light detector increases. On the other hand, perfusion index (i.e., the ratio of pulsatile signal amplitude versus DC light amplitude) can increase as the separation distance between the light emitter and light detector increases. Higher perfusion index tends to result in better rejection of noise due to motion (i.e., rejection of motion artifacts). Therefore, shorter separation distances between a light emitter and a light sensor can favor high PPG signal strength, while longer separation distances can favor high perfusion index (e.g., motion performance). That is, a trade-off can exist, making it difficult to optimize separation distance for particular user skin/tissue types and usage conditions.

Additionally, the PPG system can include several light emitters, light detectors, components, and associated wiring that may be visible to a user's eye, making the PPG system aesthetically unappealing.

SUMMARY

This relates to a PPG device configured with an architecture suitable for multiple light paths. The architecture can include one or more light emitters and one or more light sensors to generate the multiple light paths for measuring a PPG signal and a perfusion index of a user. The multiple light paths (i.e., the optical paths formed between each pair

of light emitter and light detector) can include different locations and/or emitter-to-detector separation distances to generate both an accurate PPG signal and perfusion index value to accommodate a variety of users and a variety of usage conditions. In some examples, the multiple light paths can include different path locations, but the same separation distances along each path. In other examples, the multiple light paths can include overlapping, co-linear paths (i.e., along the same line) but with different emitter-to-detector separation distances along each path. In other examples, the multiple light paths can include different path locations and different emitter-to-detector separation distances along each path. In such examples, the particular configuration of the multiple light paths can be optimized for cancellation of noise due to artifacts resulting from, for example, tilt and/or pull of the device, a user's hair, a user's skin pigmentation, and/or motion. The PPG device can further include one or more lenses and/or reflectors to increase the signal strength and/or and to obscure the light emitters, light sensors, and associated wiring from being visible to a user's eye.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A-1C illustrate systems in which examples of the disclosure can be implemented.

FIG. 2 illustrates an exemplary PPG signal.

FIG. 3A illustrates a top view and FIG. 3B illustrates a cross-sectional view of an exemplary electronic device including light sensors and light emitters for determining a heart rate signal.

FIG. 3C illustrates a flow diagram for canceling or reducing noise from a measured PPG signal.

FIG. 4A illustrates a top view and FIG. 4B illustrates a cross-sectional view of an exemplary device with two light paths for determining a heart rate signal according to examples of the disclosure.

FIG. 5A illustrates multiple light paths for determining a heart rate signal according to examples of the disclosure.

FIG. 5B illustrates a plot of PPG signal strength and perfusion index values for multiple light paths with different separation distances according to examples of the disclosure.

FIG. 6A illustrates a top view of an exemplary electronic device employing multiple light paths for determining a heart rate signal according to examples of the disclosure.

FIG. 6B illustrates a table of exemplary path lengths, relative PPG signal levels, and relative perfusion index values for an exemplary electronic device employing multiple light paths according to examples of the disclosure.

FIG. 6C illustrates a cross-sectional view of an exemplary electronic device employing multiple light paths for determining a heart rate signal according to examples of the disclosure.

FIGS. 6D-6F illustrate cross-sectional views of exemplary electronic devices employing multiple light paths for determining a heart rate signal according to examples of the disclosure.

FIG. 7A illustrates a top view of an exemplary electronic device with eight light paths for determining a heart rate signal according to examples of the disclosure.

FIG. 7B illustrates a table of light emitter/sensor paths and separation distances for an exemplary electronic device with eight light paths and four separation distances according to examples of the disclosure.

FIG. 7C illustrates a plot of PPG signal strength and perfusion index values for an exemplary architecture with eight light paths and four separation distances according to examples of the disclosure.

FIGS. 7D-7F illustrate cross-sectional views of exemplary electronic devices employing one or more light paths for determining a heart rate signal according to examples of the disclosure.

FIG. 8 illustrates an exemplary block diagram of a computing system comprising light emitters and light sensors for measuring a PPG signal according to examples of the disclosure.

FIG. 9 illustrates an exemplary configuration in which a device is connected to a host according to examples of the disclosure.

### DETAILED DESCRIPTION

In the following description of examples, reference is made to the accompanying drawings in which it is shown by way of illustration specific examples that can be practiced. It is to be understood that other examples can be used and structural changes can be made without departing from the scope of the various examples.

Various techniques and process flow steps will be described in detail with reference to examples as illustrated in the accompanying drawings. In the following description, numerous specific details are set forth in order to provide a thorough understanding of one or more aspects and/or features described or referenced herein. It will be apparent, however, to one skilled in the art, that one or more aspects and/or features described or referenced herein may be practiced without some or all of these specific details. In other instances, well-known process steps and/or structures have not been described in detail in order to not obscure some of the aspects and/or features described or referenced herein.

Further, although process steps or method steps can be described in a sequential order, such processes and methods can be configured to work in any suitable order. In other words, any sequence or order of steps that can be described in the disclosure does not, in and of itself, indicate a requirement that the steps be performed in that order. Further, some steps may be performed simultaneously despite being described or implied as occurring non-simultaneously (e.g., because one step is described after the other step). Moreover, the illustration of a process by its depiction in a drawing does not imply that the illustrated process is exclusive of other variations and modification thereto, does not imply that the illustrated process or any of its steps are necessary to one or more of the examples, and does not imply that the illustrated process is preferred.

A photoplethysmographic (PPG) signal can be measured by PPG systems to derive corresponding physiological signals (e.g., pulse rate). Such PPG systems can be designed to be sensitive to changes in blood in a user's tissue that can result from fluctuations in the amount or volume of blood or blood oxygen contained in a vasculature of the user. In a basic form, PPG systems can employ a light source or light emitter that injects light into the user's tissue and a light detector to receive light that reflects and/or scatters and exits the tissue. The PPG signal is the amplitude of the reflected and/or scattered light that is modulated with volumetric change in blood volume in the tissue. However, the PPG signal may be compromised by noise due to artifacts. Artifacts resulting from, for example, tilt and/or pull of the device relative to the user's tissue, hair, and/or motion can introduce noise into the signal. For example, the amplitude

of reflected light can modulate due to the motion of the user's hair. As a result, the amplitude modulation of the reflected light caused by hair motion can be erroneously interpreted as a result of pulsatile blood flow.

This disclosure relates to a multiple light paths architecture and obscuration methods for PPG signal and perfusion index optimization. The architecture can include one or more light emitters and one or more light sensors to generate the multiple light paths to measure a PPG signal and a perfusion index of a user. The multiple light paths can include different locations and/or separation distances between light emitters and light detectors to generate both an accurate PPG signal and perfusion index value to accommodate a variety of users and a variety of usage conditions. In some examples, the multiple light paths can include different path locations, but the same emitter-to-detector separation distances along each path. In some examples, the multiple light paths can include overlapping, co-linear paths (i.e., along the same line), but with different emitter-to-detector separation distances along each other. In some examples, the multiple light paths can include different path locations and different emitter-to-detector separation distances along each path. In such examples, the particular configuration of the multiple light paths is optimized for noise cancellation due to artifacts such as tilt and/or pull of the device, a user's hair, a user's skin pigmentation, and/or motion. In some examples, the device can include one or more lenses and/or reflectors to increase the signal strength and/or to obscure the light emitters, light sensors, and associated wiring from being visible to a user's eye.

Representative applications of methods and apparatus according to the present disclosure are described in this section. These examples are being provided solely to add context and aid in the understanding of the described examples. It will thus be apparent to one skilled in the art that the described examples may be practiced without some or all of the specific details. In other instances, well-known process steps have been described in detail in order to avoid unnecessarily obscuring the described examples. Other applications are possible, such that the following examples should not be taken as limiting.

FIGS. 1A-1C illustrate systems in which examples of the disclosure can be implemented. FIG. 1A illustrates an exemplary mobile telephone **136** that can include a touch screen **124**. FIG. 1B illustrates an exemplary media player **140** that can include a touch screen **126**. FIG. 1C illustrates an exemplary wearable device **144** that can include a touch screen **128** and can be attached to a user using a strap **146**. The systems of FIGS. 1A-1C can utilize the multiple light path architectures and obscuration methods as will be disclosed.

FIG. 2 illustrates an exemplary PPG signal. A user's PPG signal absent of artifacts is illustrated as signal **210**. However, movement of the body of the user can cause the skin and vasculature to expand and contract, introducing noise to the signal. Additionally, a user's hair and/or tissue can change the amplitude of light reflected and the amplitude of light absorbed. A user's PPG signal with artifacts is illustrated as signal **220**. Without extraction of noise, signal **220** can be misinterpreted.

Signal **210** can include light information with an amplitude that is modulated as a result of pulsatile blood flow (i.e., "signal") and parasitic, unmodulated, non-signal light (i.e., DC). From the measured PPG signal **210**, a perfusion index can be determined. The perfusion index can be the ratio of received modulated light (ML) to unmodulated light (UML) (i.e., ratio of blood flow modulated signal to static, parasitic

DC signal) and can give extra information regarding the user's physiological state. The modulated light (ML) can be the peak-to-valley value of signal **210**, and unmodulated light (UML) can be the zero-to-average (using average **212**) value of signal **210**. As shown in FIG. 2, the perfusion index can be equal to the ratio of ML to UML.

Both the PPG signal and perfusion index can be related to an accurate measurement of physiological signals such as heart rate. However, the PPG signal can include noise from modulated light resulting from, for example, motion of the user's tissue and/or the PPG device. Higher perfusion index (e.g., higher pulsatile signal and/or lower parasitic DC) can result in better rejection of such motion noise. Additionally, the intensity of a PPG signal relative to perfusion index can vary for different users. Some users may naturally have a high PPG signal, but a weak perfusion index or vice versa. Thus, the combination of PPG signal and perfusion index can be used to determine physiological signals for a variety of users and a variety of usage conditions.

FIG. 3A illustrates a top view and FIG. 3B illustrates a cross-sectional view of an exemplary electronic device including light sensors and light emitters for determining a heart rate signal. A light sensor **304** can be located with a light emitter **306** on a surface of device **300**. Additionally, another light sensor **314** can be located or paired with light emitter **316** on a surface of device **300**. Device **300** can be situated such that light sensors **304** and **314** and light emitters **306** and **316** are proximate to a skin **320** of a user. For example, device **300** can be held in a user's hand or strapped to a user's wrist, among other possibilities.

Light emitter **306** can generate light **322**. Light **322** can be incident on skin **320** and can reflect back to be detected by light sensor **304**. A portion of light **322** can be absorbed by skin **320**, vasculature, and/or blood, and a portion of light (i.e., light **332**) can be reflected back to light sensor **304** located or paired with light emitter **306**. Similarly, light emitter **316** can generate light **324**. Light **324** can be incident on skin **320** and can reflect back to be detected by light sensor **314**. A portion of light **324** can be absorbed by skin **320**, vasculature, and/or blood, and a portion of light (i.e., light **334**) can be reflected back to light sensor **314** located with light emitter **316**. Light **332** and **334** can include information or signals such as a heart rate signal (i.e., PPG signal) due to a blood pulse wave **326**. Due to a distance between light sensors **304** and **314** along the direction of the blood pulse wave **326**, signal **332** can include a heart rate signal, whereas signal **334** can include a time-shifted heart rate signal. A difference between signal **332** and signal **334** can depend on the distance between light sensors **304** and **314** and the velocity of blood pulse wave **326**.

Signals **332** and **334** can include noise **312** due to artifacts resulting from, for example, tilt and/or pull of device **300** relative to skin **320**, a user's hair, and/or a user's motion. One way to account for noise **312** can be to locate light sensors **304** and **314** far enough such that noise in signals **332** and **334** may be uncorrelated, but close enough together that PPG signal is corrected in signals **332** and **334**. The noise can be mitigated by scaling, multiplying, dividing, adding, and/or subtracting signals **332** and **334**.

FIG. 3C illustrates a flow diagram for canceling or reducing noise from a measured PPG signal. Process **350** can include light emitted from one or more light emitters **306** and **316** (step **352**) located on a surface of device **300**. Light information **332** can be received by light sensor **304** (step **354**), and light information **334** can be received by light sensor **314** (step **356**). In some examples, light information **332** and **334** can indicate an amount of light from light

emitters **306** and **316** that has been reflected and/or scattered by skin **320**, blood, and/or vasculature of the user. In some examples, light information **332** and **334** can indicate an amount of light that has been absorbed by skin **320**, blood, and/or vasculature of the user.

Based on light information **332** and light information **334**, a heart rate signal can be computed by canceling noise due to artifacts (step **358**). For example, light information **334** can be multiplied by a scaling factor and added to light information **332** to obtain the heart rate signal. In some examples, heart rate signal can be computed by merely subtracting or dividing light information **334** from light information **332**.

In some examples, light information **332** and **334** can be difficult to determine due to a low signal intensity. To increase the signal intensity or signal strength, the distance between light sensors and light emitters can be reduced or minimized such that light travels the shortest distance. Generally, for a given light emitter and light sensor pair, the signal strength decreases with increasing separation distance between the light emitter and light sensor. On the other hand, the perfusion index generally increases with increasing separation distance between the light emitter and the light sensor. A higher perfusion index can correlate to better rejection of artifacts caused by, for example, motion. Therefore, shorter separation distances between a light emitter and a light sensor can favor high PPG signal strength, while longer separation distances can favor high perfusion index (e.g., motion performance). That is, a trade-off can exist making it difficult to optimize separation distance for particular user skin/tissue types and usage conditions.

To alleviate the trade-off issue between signal strength and perfusion index, multiple light paths with various distances between light emitter(s) and light sensor(s) can be employed. FIG. 4A illustrates a top view and FIG. 4B illustrates a cross-sectional view of an exemplary device with two light paths for determining a heart rate signal according to examples of the disclosure. Device **400** can include light emitters **406** and **416** and a light sensor **404**. Light emitter **406** can have a separation distance **411** from light sensor **404**, and light emitter **416** can have a separation distance **413** from light sensor **404**.

Light **422** from light emitter **406** can be incident on skin **420** and can reflect back as light **432** to be detected by light sensor **404**. Similarly, light **424** from light emitter **416** can be incident on skin **420** and can reflect back as light **434** to be detected by light sensor **404**. Separation distance **411** can be small compared to separation distance **413**, and as a result, light information **432** can have a higher PPG signal strength than light information **434**. Light information **432** can be employed for applications requiring a higher PPG signal strength. Separation distance **413** can be large compared to separation distance **411**, and as a result, light information **434** can have a higher perfusion index than light information **432**. Light information **434** can be employed for applications requiring a high perfusion index (e.g., motion performance). Due to the different separation distances **411** and **413**, light information **432** and **434** can provide various combinations of PPG signals and perfusion index values to allow the device to dynamically select light information for particular user skin types and usage conditions (e.g., sedentary, active motion, etc.).

FIG. 5A illustrates multiple light paths for determining a heart rate signal according to examples of the disclosure. For enhanced measurement resolution, more than two light paths can be employed. Multiple light paths can be formed from a light emitter **506** and a plurality of light sensors such as

light sensors **504**, **514**, **524**, **534**, and **544**. Light sensor **504** can have a separation distance **511** from light emitter **506**. Light sensor **514** can have a separation distance **513** from light emitter **506**. Light sensor **524** can have a separation distance **515** from light emitter **506**. Light sensor **534** can have a separation distance **517** from light emitter **506**. Light sensor **544** can have a separation distance **519** from light emitter **506**. Separation distances **511**, **513**, **515**, **517**, and **519** can be different values.

FIG. **5B** illustrates a plot of PPG signal strength and perfusion index values for light emitter **506** and light sensors **504**, **514**, **524**, **534**, and **544**. As shown, an intensity of the PPG signal or signal strength can decrease as the separation distance between a light emitter and a light sensor (i.e., separation distances **511**, **513**, **515**, **517**, and **519**) increases. On the other hand, the perfusion index value can increase as the separation distance between a light emitter and a light sensor increases.

Information obtained from the multiple light paths can be used both for applications requiring a high PPG signal strength and applications requiring a high perfusion index value. In some examples, information generated from all light paths can be utilized. In some examples, information generated from some, but not all light paths can be utilized. In some examples, the “active” light paths can be dynamically changed based on the application(s), available power, user type, and/or measurement resolution.

FIG. **6A** illustrates a top view and FIG. **6C** illustrates a cross-sectional view of an exemplary electronic device employing multiple light paths for determining a heart rate signal according to examples of the disclosure. Device **600** can include light emitters **606** and **616** and light sensors **604** and **614** located on a surface of device **600**. Light sensors **604** and **614** can be symmetrically placed, while light emitters **606** and **616** can be asymmetrically placed. Optical isolation **644** can be disposed between light emitters **606** and **616** and light detectors **604** and **614**. In some examples, optical isolation **644** can be an opaque material to, for example, reduce parasitic DC light.

Light emitters **606** and **616** and light sensors **604** and **614** can be mounted on or touching component mounting plane **648**. In some examples, component mounting plane **648** can be made of an opaque material (e.g., flex). In some examples, component mounting plane **648** can be made of a same material as optical isolation **644**.

Device **600** can include windows **601** to protect light emitters **606** and **616** and light sensors **604** and **614**. Light emitters **606** and **616**, light detectors **604** and **614**, optical isolation **644**, component mounting plane **648**, and windows **601** can be located within an opening **603** of housing **610**. In some examples, device **600** can be a wearable device such as a wristwatch, and housing **610** can be coupled to a wrist strap **646**.

Light emitters **606** and **616** and light detectors **604** and **614** can be arranged such that there are four light paths with four different separation distances. Light path **621** can be coupled to light emitter **606** and light sensor **604**. Light path **623** can be coupled to light emitter **606** and light sensor **614**. Light path **625** can be coupled to light emitter **616** and light sensor **614**. Light path **627** can be coupled to light emitter **616** and light sensor **604**.

FIG. **6B** illustrates a table of exemplary path lengths, relative PPG signals levels, and relative perfusion index values for light paths **621**, **623**, **625**, and **627** of device **600** according to examples of the disclosure. As shown, relative PPG signal levels can have higher values for shorter path lengths. For example, light path **625** can have a higher PPG

signal of 1.11 than light path **627** with a PPG signal of 0.31 due to the shorter path length (i.e., path length of light path **625** is 4.944 mm, whereas path length of light path **627** is 6.543 mm). For applications that require high PPG signal levels, device **600** can utilize information from light path **625** or light path **621**. However, relative perfusion index values can have higher values for longer path lengths. For example, light path **623** can have a higher perfusion index value of 1.23 than light path **621** with a perfusion index value of 1.10 due to the longer path length (e.g., path length of light path **623** is 5.915 mm, whereas path length of light path **621** is 5.444 mm). For applications that require high perfusion index values, device **600** can favor information from light path **623** over information from light path **621**. While FIG. **6B** illustrates exemplary values for path lengths **621**, **623**, **625**, and **627** along with exemplary PPG signal levels and perfusion index values, examples of the disclosure are not limited to these values.

FIGS. **6D-6F** illustrate cross-sectional views of exemplary electronic devices employing multiple light paths for determining a heart rate signal according to examples of the disclosure. As shown in FIG. **6D**, optical isolation **654** can be designed to improve mechanical stability of device **600** by providing a larger surface area (than optical isolation **644** of FIG. **6C**) for windows **601** to rest on and/or adhere to. While optical isolation **654** can provide a larger surface area for windows **601**, the light may have to travel a longer distance through skin **620**, and as a result, the signal intensity may be reduced. Either the signal quality can be compromised or device **600** can compensate by increasing the power (i.e., battery power consumption) of light emitted from light emitter **606**. A lower signal intensity or a higher battery power consumption can degrade the user’s experience.

One way to overcome the issues with lower signal intensity and higher power consumption can be illustrated in FIG. **6E**. Device **600** can include lens **609** coupled to light emitter **606** and/or lens **605** coupled to light sensor **604**. Lens **609** can be any type of lens such as a Fresnel lens or image displacement film (IDF) that steers the light over the optical isolation **644**. Lens **605** can be any type of lens such as an IDF or a brightness enhancement film (BEF) that shifts the light into an optical receiving area of light sensor **604**. Lens **609** can direct light emitted from light emitter **606** closer to lens **605**, and lens **605** can direct light to closer light sensor **604**. By employing lenses **609** and/or **605**, light may not have to travel a longer distance through skin **620**, and as a result, the signal intensity can be recovered.

In some examples, device **600** can include a reflector **607**, in addition to or alternatively to lens **609** and **605**, as shown in FIG. **6F**. Reflector **607** can be formed from any reflective material such as a mirror or a white surface. Light emitted from light emitter **606** can reflect off the surface of skin **620** and be directed back to reflector **607**. Such light in the architectures illustrated in FIGS. **6D-6E** could be lost or absorbed by optical isolation **654**. However, in the architecture illustrated in FIG. **6F**, reflector **607** can prevent light loss by reflecting the light back to skin **620**, and the light could then be reflected to light sensor **604**. In some examples, optical isolation **654** can include any number of reflectors **607**. In some examples, one or more windows **601** can include any number of reflectors **607**.

FIG. **7A** illustrates a top view of an exemplary electronic device with multiple light paths for determining a heart rate signal according to examples of the disclosure. Device **700** can include a plurality of light emitters **706** and **716** and a plurality of light sensors **704**, **714**, **724**, and **734** located on

a surface of device 700. Optical isolation 744 can be disposed between light emitters 706 and 716 and light sensors 704, 714, 724, and 734 to prevent light mixing. Component mounting plane 748 can be mounted behind light emitters 706 and 716 and light sensors 704, 714, 724, and 734. Windows such as window 701 can be located in front of light emitters 706 and 716 and light sensors 704, 714, 724, and 734 for protection. The plurality of light emitters 706 and 716, plurality of light detectors 704, 714, 724, and 734, optical isolation 744, component mounting plane 748, and windows 701 can be located within an opening 703 of housing 710. In some examples, device 700 can be a wearable device such as a wristwatch, and housing 710 can be coupled to a wrist strap 746.

Although FIG. 7A illustrates two light emitters and four light sensors, any number of light emitters and light sensors can be employed. In some examples, light sensors 704 and 724 can be a single light sensor partitioned into two or more separate sensing regions. Similarly, light sensors 714 and 734 can be a single light sensor partitioned into two or more separate sensing regions. In some examples, optical isolation 744 and/or component mounting plane 748 can be an opaque material. In some examples, one or more of optical isolation 744, component mounting plane 748, and housing 710 can be a same material.

Light emitters 706 and 716 and light sensors 704, 714, 724, and 734 can be arranged such that there are eight light paths with four different path lengths or separation distances. Light path 721 can be coupled to light emitter 706 and light sensor 704. Light path 723 can be coupled to light emitter 706 and light sensor 734. Light path 725 can be coupled to light emitter 706 and light sensor 714. Light path 727 can be coupled to light emitter 716 and light sensor 734. Light path 729 can be coupled to light emitter 716 and light sensor 714. Light path 731 can be coupled to light emitter 716 and light sensor 724. Light path 733 can be coupled to light emitter 716 and light sensor 704. Light path 735 can be coupled to light emitter 706 and light sensor 724.

Light emitters 706 and 716 and light sensors 704, 714, 724, and 734 can be placed such that the separation distances of light paths 721 and 729 (i.e., separation distance d1) are the same, the separation distances of light paths 727 and 735 (i.e., separation distance d2) are the same, the separation distances of light paths 723 and 731 (i.e., separation distance d3) are the same, and the separation distances of light paths 725 and 733 (i.e., separation distance d4) are the same. In some examples, two or more of the light paths can be overlapping light paths. In some examples, two or more of the light paths can be non-overlapping light paths. In some examples, two or more light paths can be co-located light paths. In some examples, two or more light paths can be non-co-located light paths.

An advantage to the multiple light-path architecture illustrated in FIG. 7A can be signal optimization. There can be non-overlapping light paths such that if there is signal loss in one light path, other light paths can be used for signal redundancy. That is, the device can ensure the existence of a signal by having light paths that collectively span a larger total area. The architecture can mitigate against the risk of having only one light path where signal is either very low or non-existent. A very low or non-existent signal can render a light path ineffective due to, for example, a user's particular physiology where a "quiet" no-signal (or low signal) spot exists. For example, light path 729 can be used for signal redundancy when there is signal loss in light path 721.

FIG. 7B illustrates a table of light emitter/sensor paths and separation distances for an exemplary electronic device with

eight light paths and four separation distances according to examples of the disclosure. FIG. 7C illustrates a plot of PPG signal strength and perfusion index values for an exemplary architecture with eight light paths and four separation distances according to examples of the disclosure. As shown, an intensity of the PPG signal can decrease as the separation distance between a light emitter and a light sensor (i.e., separation distances d1, d2, d3, and d4) increases. On the other hand, the perfusion index value can increase as the separation distance between a light emitter and a light sensor increases.

By configuring the light sensors and light emitters such that multiple light paths have a same separation distance, noise due to artifacts such as motion, user hair and user skin can be canceled or reduced. For example, light path 721 and light path 729 can be two different light paths with a same separation distance d1. Due to the separation distance being the same for both light paths, the PPG signal should be the same. However, light path 721 can reflect off a different area of the user's skin, vasculature, and blood than light path 729. Due to the asymmetry of the human skin, vasculature, and blood, light information from light path 721 can be different than light information from light path 729. For example, a user's skin pigmentation in light path 721 can be different than the user's skin pigmentation in light path 729, leading to a different signal for light path 721 and light path 729. Such differences in light information can be used to cancel or reduce noise and/or enhance pulsatile signal quality to determine an accurate PPG signal.

In some examples, light emitters 706 and 716 can be different light sources. Exemplary light sources can include, but are not limited to, light emitting diodes (LEDs), incandescent lights, and fluorescent lights. In some examples, light emitters 706 and 716 can have different emission wavelengths. For example, light emitter 706 can be a green LED and light emitter 716 can be an infrared (IR) LED. A user's blood can effectively absorb light from a green light source, and thus, the light path coupled to light emitter 706 with the shortest separation distance (i.e., light path 721) can be used for a high PPG signal when a user is sedentary, for example. An IR light source can effectively travel further distances through a user's skin than other light sources and as a result, can consume less power. A light path coupled to light emitter 716 (i.e., light paths 727, 729, 731, and 733) can be used when device 700 is operating in a low power mode, for example. In some examples, light emitters 706 and 716 can have different emission intensities.

FIGS. 7D-7F illustrate cross-sectional views of exemplary electronic devices employing one or more light paths for determining a heart rate signal according to examples of the disclosure. Device 700 can include window 701 located in front of a component such as light emitter 706 of FIG. 7D and light sensor 704 of FIG. 7E. Window 701 may be transparent, and as a result, the internal components of device 700 may be visible to a user. Since device 700 can include several components and associated wiring, it can be desirable to obscure the components and prevent internal components from being visible to a user's eye. In addition to obscuring the internal components, it may be desirable that the light emitted from light emitter 706 retains its optical power, collection efficiency, beam shape, and collection area so that the intensity of light is unaffected.

To obscure internal components, a lens such as a Fresnel lens 707 can be located between window 701 and light emitter 706, as shown in FIG. 7D. Fresnel lens 707 can have two regions: an optical center 709 and a cosmetic zone 711. Optical center 709 can be placed in substantially a same area

## 11

or location as light emitter **706** to collimate the emitted light into a smaller beam size. Cosmetic zone **711** can be located in areas outside of optical center **709**. The ridges of the cosmetic zone **709** can act to obscure the underlying internal components.

To obscure light sensor **704**, a lens such as Fresnel lens **713** can be located between window **701** and light sensor **704**, as shown in FIG. 7E. Because light sensor **704** can be a large-area photodiode, shaping of the light field may not be needed, so Fresnel lens **713** may not require an optical center. Instead, Fresnel lens **713** may have one region comprising ridges configured for a cosmetic zone.

The ridge shapes of Fresnel lenses **707** and **713** can be altered to improve obscuration, especially in cosmetic zones. For example, deep and sharp sawtooth patterns can be used for high obscuration needs. Other types of ridge shapes can include rounded cylindrical ridges, asymmetric shapes, and wavy shapes (i.e., ridges that move in and out).

In some examples, the Fresnel lens **707** illustrated in FIG. 7D can be used additionally or alternatively for light collimation. By collimating light, the optical signal efficiency can be improved. Without a lens or similar collimating optical element, emitter light can be directed at an angle away from the light sensor and can be lost. Additionally or alternatively, light can be directed at an angle toward the light sensor, but the angle may be shallow. The shallow angle may prevent the light from penetrating deep enough to reach the signal layers in the skin. This light may contribute only to parasitic, non-signal light. The Fresnel lens **707** can redirect light to directions that otherwise may be lost or enter into the tissue at shallow angles. Such redirected light can be collected instead of being lost and/or can mitigate against parasitic non-signal light, resulting in improved optical signal efficiency.

In some examples, a diffusing agent can be used. Diffusing agent **719** can be surrounding, touching, and/or covering one or more components of light emitter **706**. In some examples, diffusing agent **719** can be a resin or epoxy that encapsulates the dies or components and/or wire bonds. Diffusing agent **719** can be used to adjust the angle of the light emitted from light emitter **706**. For example, the angle of light emitted from a light emitter without a diffusing agent can be 5° wider than the angle of light emitter from light emitter **706** encapsulated by diffusing agent **719**. By narrowing the beam of light emitted, more light can be collected by the lens and/or window resulting in a larger amount of detected light by the light sensor.

In some examples, diffusing agent **719** can have an increased reflectivity for the wavelength or color of emitted light from light emitter **706**. For example, if light emitter **706** emits green light, diffusing agent **719** can be made of white TiO<sub>2</sub> material to increase the amount of green light reflected back toward the skin. This way, light that would have otherwise been lost can be recycled back and detected by the light detector.

FIG. 8 illustrates an exemplary block diagram of a computing system comprising light emitters and light sensors for measuring a PPG signal according to examples of the disclosure. Computing system **800** can correspond to any of the computing devices illustrated in FIGS. 1A-1C. Computing system **800** can include a processor **810** configured to execute instructions and to carry out operations associated with computing system **800**. For example, using instructions retrieved from memory, processor **810** can control the reception and manipulation of input and output data between

## 12

components of computing system **800**. Processor **810** can be a single-chip processor or can be implemented with multiple components.

In some examples, processor **810** together with an operating system can operate to execute computer code and produce and use data. The computer code and data can reside within a program storage block **802** that can be operatively coupled to processor **810**. Program storage block **802** can generally provide a place to hold data that is being used by computing system **800**. Program storage block **802** can be any non-transitory computer-readable storage medium, and can store, for example, history and/or pattern data relating to PPG signal and perfusion index values measured by one or more light sensors such as light sensor **804**. By way of example, program storage block **802** can include Read-Only Memory (ROM) **818**, Random-Access Memory (RAM) **822**, hard disk drive **808** and/or the like. The computer code and data could also reside on a removable storage medium and loaded or installed onto the computing system **800** when needed. Removable storage mediums include, for example, CD-RM, DVD-ROM, Universal Serial Bus (USB), Secure Digital (SD), Compact Flash (CF), Memory Stick, Multi-Media Card (MMC) and a network component.

Computing system **800** can also include an input/output (I/O) controller **812** that can be operatively coupled to processor **810** or it may be a separate component as shown. I/O controller **812** can be configured to control interactions with one or more I/O devices. I/O controller **812** can operate by exchanging data between processor **810** and the I/O devices that desire to communicate with processor **810**. The I/O devices and I/O controller **812** can communicate through a data link. The data link can be a one way link or a two way link. In some cases, I/O devices can be connected to I/O controller **812** through wireless connections. By way of example, a data link can correspond to PS/2, USB, Firewire, IR, RF, Bluetooth or the like.

Computing system **800** can include a display device **824** that can be operatively coupled to processor **810**. Display device **824** can be a separate component (peripheral device) or can be integrated with processor **810** and program storage block **802** to form a desktop computer (all in one machine), a laptop, handheld or tablet computing device of the like. Display device **824** can be configured to display a graphical user interface (GUI) including perhaps a pointer or cursor as well as other information to the user. By way of example, display device **824** can be any type of display including a liquid crystal display (LCD), an electroluminescent display (ELD), a field emission display (FED), a light emitting diode display (LED), an organic light emitting diode display (OLED) or the like.

Display device **824** can be coupled to display controller **826** that can be coupled to processor **810**. Processor **810** can send raw data to display controller **826**, and display controller **826** can send signals to display device **824**. Data can include voltage levels for a plurality of pixels in display device **824** to project an image. In some examples, processor **810** can be configured to process the raw data.

Computing system **800** can also include a touch screen **830** that can be operatively coupled to processor **810**. Touch screen **830** can be a combination of sensing device **832** and display device **824**, where the sensing device **832** can be a transparent panel that is positioned in front of display device **824** or integrated with display device **824**. In some cases, touch screen **830** can recognize touches and the position and magnitude of touches on its surface. Touch screen **830** can report the touches to processor **810**, and processor **810** can interpret the touches in accordance with its programming.

For example, processor **810** can perform tap and event gesture parsing and can initiate a wake of the device or powering on one or more components in accordance with a particular touch.

Touch screen **830** can be coupled to a touch controller **840** that can acquire data from touch screen **830** and can supply the acquired data to processor **810**. In some cases, touch controller **840** can be configured to send raw data to processor **810**, and processor **810** processes the raw data. For example, processor **810** can receive data from touch controller **840** and can determine how to interpret the data. The data can include the coordinates of a touch as well as pressure exerted. In some examples, touch controller **840** can be configured to process raw data itself. That is, touch controller **840** can read signals from sensing points **834** located on sensing device **832** and turn them into data that the processor **810** can understand.

Touch controller **840** can include one or more microcontrollers such as microcontroller **842**, each of which can monitor one or more sensing points **834**. Microcontroller **842** can, for example, correspond to an application specific integrated circuit (ASIC), which works with firmware to monitor the signals from sensing device **832**, process the monitored signals, and report this information to processor **810**.

One or both display controller **826** and touch controller **840** can perform filtering and/or conversion processes. Filtering processes can be implemented to reduce a busy data stream to prevent processor **810** from being overloaded with redundant or non-essential data. The conversion processes can be implemented to adjust the raw data before sending or reporting them to processor **810**.

In some examples, sensing device **832** is based on capacitance. When two electrically conductive members come close to one another without actually touching, their electric fields can interact to form a capacitance. The first electrically conductive member can be one or more of the sensing points **834**, and the second electrically conductive member can be an object **890** such as a finger. As object **890** approaches the surface of touch screen **830**, a capacitance can form between object **890** and one or more sensing points **834** in close proximity to object **890**. By detecting changes in capacitance at each of the sensing points **834** and noting the position of sensing points **834**, touch controller **840** can recognize multiple objects, and determine the location, pressure, direction, speed and acceleration of object **890** as it moves across the touch screen **830**. For example, touch controller **840** can determine whether the sensed touch is a finger, tap, or an object covering the surface.

Sensing device **832** can be based on self-capacitance or mutual capacitance. In self-capacitance, each of the sensing points **834** can be provided by an individually charged electrode. As object **890** approaches the surface of the touch screen **830**, the object can capacitively couple to those electrodes in close proximity to object **890**, thereby stealing charge away from the electrodes. The amount of charge in each of the electrodes can be measured by the touch controller **840** to determine the position of one or more objects when they touch or hover over the touch screen **830**. In mutual capacitance, sensing device **832** can include a two layer grid of spatially separated lines or wires, although other configurations are possible. The upper layer can include lines in rows, while the lower layer can include lines in columns (e.g., orthogonal). Sensing points **834** can be provided at the intersections of the rows and columns. During operation, the rows can be charged, and the charge can capacitively couple from the rows to the columns. As

object **890** approaches the surface of the touch screen **830**, object **890** can capacitively couple to the rows in close proximity to object **890**, thereby reducing the charge coupling between the rows and columns. The amount of charge in each of the columns can be measured by touch controller **840** to determine the position of multiple objects when they touch the touch screen **830**.

Computing system **800** can also include one or more light emitters such as light emitters **806** and **816** and one or more light sensors such as light sensor **804** proximate to skin **820** of a user. Light emitters **806** and **816** can be configured to generate light, and light sensor **804** can be configured to measure a light reflected or absorbed by skin **820**, vasculature, and/or blood of the user. Light sensor **804** can send measured raw data to processor **810**, and processor **810** can perform noise cancelation to determine the PPG signal and/or perfusion index. Processor **810** can dynamically activate light emitters and/or light sensors based on an application, user skin type, and usage conditions. In some examples, some light emitters and/or light sensors can be activated, while other light emitters and/or light sensors can be deactivated to conserve power, for example. In some examples, processor **810** can store the raw data and/or processed information in a ROM **818** or RAM **822** for historical tracking or for future diagnostic purposes.

In some examples, the light sensor(s) can measure light information and a processor can determine a PPG signal and/or perfusion index from the reflected, scattered, or absorbed light. Processing of the light information can be performed on the device as well. In some examples, processing of light information need not be performed on the device itself. FIG. **9** illustrates an exemplary configuration in which a device is connected to a host according to examples of the disclosure. Host **910** can be any device external to device **900** including, but not limited to, any of the systems illustrated in FIGS. **1A-1C** or a server. Device **900** can be connected to host **910** through communications link **920**. Communications link **920** can be any connection including, but not limited to, a wireless connection and a wired connection. Exemplary wireless connections include Wi-Fi, Bluetooth, Wireless Direct, and Infrared. Exemplary wired connections include Universal Serial Bus (USB), FireWire, Thunderbolt, or any connection requiring a physical cable.

In operation, instead of processing light information from the light sensors on the device **900** itself, device **900** can send raw data **930** measured from the light sensors over communications link **920** to host **910**. Host **910** can receive raw data **930**, and host **910** can process the light information. Processing the light information can include canceling or reducing any noise due to artifacts and determining physiological signals such as a user's heart rate. Host **910** can include algorithms or calibration procedures to account for differences in a user's characteristics affecting PPG signal and perfusion index. Additionally, host **910** can include storage or memory for tracking a PPG signal and perfusion index history for diagnostic purposes. Host **910** can send the processed result **940** or related information back to device **900**. Based on the processed result **940**, device **900** can notify the user or adjust its operation accordingly. By offloading the processing and/or storage of the light information, device **900** can conserve space and power enabling device **900** to remain small and portable, as space that could otherwise be required for processing logic can be freed up on the device.

In some examples, an electronic device is disclosed. The electronic device may comprise: one or more light emitters configured to generate a plurality of light paths, wherein at

least two of the plurality of light paths have separation distances with a predetermined relationship; one or more light sensors configured to detect the at least two light paths having the predetermined relationship; and logic coupled to the one or more light sensors and configured to detect a physiological signal from the at least two light paths. Additionally or alternatively to one or more examples disclosed above, in other examples, the predetermined relationship is a same separation distance. Additionally or alternatively to one or more examples disclosed above, in other examples, the logic is further configured to generate PPG signals and perfusion signals from the detected physiological signal. Additionally or alternatively to one or more examples disclosed above, in other examples, the predetermined relationship is different separation distances. Additionally or alternatively to one or more examples disclosed above, in other examples, the predetermined relationship is overlapping light paths. Additionally or alternatively to one or more examples disclosed above, the predetermined relationship is non-overlapping light paths. Additionally or alternatively to one or more examples disclosed above, in other examples, the predetermined relationship is co-located light paths. Additionally or alternatively to one or more examples disclosed above, in other examples, the predetermined relationship is non-co-located light paths. Additionally or alternatively to one or more examples disclosed above, in other examples, the logic is further configured to reduce noise in the plurality of light paths. Additionally or alternatively to one or more examples disclosed above, in other examples, the electronic device further comprises one or more first lenses disposed on the one or more light emitters. Additionally or alternatively to one or more examples disclosed above, in other examples, at least one of the one or more first lenses is a Fresnel lens or an image displacement film. Additionally or alternatively to one or more examples disclosed above, in other examples, at least one of the one or more first lenses includes an optical center placed in substantially a same location as light emitted from the one or more light emitters. Additionally or alternatively to one or more examples disclosed above, in other examples, the electronic device further comprises one or more second lenses disposed on the one or more light sensors. Additionally or alternatively to one or more examples disclosed above, in other examples, at least one of the one or more second lenses is an image displacement film, a brightness enhancement film, or a Fresnel lens. Additionally or alternatively to one or more examples disclosed above, in other examples, the electronic device further comprises: an optical isolation disposed between the one or more light emitters and the one or more light sensors; and a reflector disposed on at least one of the optical isolation, a window disposed on the one or more light emitters, and a window disposed on the one or more light sensors. Additionally or alternatively to one or more examples disclosed above, in other examples, at least one light sensor is partitioned into a plurality of sensing regions. Additionally or alternatively to one or more examples disclosed above, in other examples, at least two of the one or more light emitters emit light at different wavelengths. Additionally or alternatively to one or more examples disclosed above, in other examples, at least one light emitter is a green light emitting diode and at least one light emitter is an infrared light emitting diode.

In some examples, a method for forming an electronic device including one or more light emitters and one or more light sensors is disclosed. The method may comprise: emitting light from the one or more light emitters to generate a plurality of light paths, wherein at least two of the plurality

of light paths have separation distances with a predetermined relationship; receiving light from the one or more light sensors; and determining a physiological signal from the received light. Additionally or alternatively to one or more examples disclosed above, in other examples, the method further comprises dynamically selecting one or more light paths based on at least one of a user characteristic and a usage condition. Additionally or alternatively to one or more examples disclosed above, in other examples, at least two of the plurality of light paths have a same separation distance, the method further comprises canceling or reducing a noise from the at least two of the plurality of light paths with the same separation distance. Additionally or alternatively to one or more examples disclosed above, in other examples, the at least two of the plurality of light paths including a first light path and a second light path, wherein the first light path has a first separation distance and the second light path has a second separation distance, and the first separation distance is shorter than the second separation distance, the method further comprises: determining a first physiological signal from the first light path; and determining a second physiological signal from the second light path. Additionally or alternatively to one or more examples disclosed above, in other examples, the first physiological signal is indicative of a photoplethysmographic signal and the second physiological signal is indicative of a perfusion index. Additionally or alternatively to one or more examples disclosed above, in other examples, the one or more light emitters includes a first set of light emitters and a second set of light emitters, the method further comprising: dynamically activating the first set of light emitters; and dynamically deactivating the second set of light emitters.

Although the disclosed examples have been fully described with reference to the accompanying drawings, it is to be noted that various changes and modifications will become apparent to those skilled in the art. Such changes and modifications are to be understood as being included within the scope of the disclosed examples as defined by the appended claims.

The invention claimed is:

1. A wearable electronic device comprising:

- a first window;
- a first light sensor positioned behind the first window;
- a second window;
- a second light sensor positioned behind the second window;
- a third window;
- a first emitter positioned behind and off-center with respect to the third window;
- a second emitter positioned behind the third window; and
- a first Fresnel lens positioned between the first emitter and the third window and comprising:
  - a first zone that is positioned above the first emitter and configured to collimate light emitted by the first emitter; and
  - a second zone that is positioned above the second emitter and includes ridges that act to obscure components underlying the second zone.

2. The wearable electronic device of claim 1, wherein:
 

- the first light sensor is centered within the first window; and
- the second light sensor is centered within the second window.

3. The wearable electronic device of claim 1, further comprising:
 

- a second Fresnel lens positioned between the first window and the first light sensor.



17

4. The wearable electronic device of claim 1, wherein the first emitter and the second emitter have different emission wavelengths.

5. The wearable electronic device of claim 4, wherein the first emitter is a green LED.

6. The wearable electronic device of claim 5, wherein the second emitter is an infrared LED.

7. The wearable electronic device of claim 1, comprising a third light sensor positioned behind the first window.

8. The wearable electronic device of claim 7, comprising a fourth light sensor positioned behind the second window.

9. A wearable electronic device comprising:

a first window;

a first light sensor positioned behind the first window;

a second window;

a second light sensor positioned behind the second window;

a third window;

a first emitter positioned behind the third window;

a second emitter positioned behind the third window;

a first Fresnel lens positioned between the first emitter and the third window and comprising:

a first zone that is positioned above the first emitter and configured to collimate light emitted by the first emitter; and

a second zone that is positioned above the second emitter and includes ridges that act to obscure components underlying the second zone; and

a second Fresnel lens positioned between the first light sensor and the first window.

10. The wearable electronic device of claim 9, wherein: the first light sensor is centered within the first window; and

the second light sensor is centered within the second window.

11. The wearable electronic device of claim 9, wherein the first emitter and the second emitter have different emission wavelengths.

12. The wearable electronic device of claim 11, wherein the first emitter is a green LED.

13. The wearable electronic device of claim 12, wherein the second emitter is an infrared LED.

14. The wearable electronic device of claim 9, comprising a third light sensor positioned behind the first window.

15. The wearable electronic device of claim 14, comprising a fourth light sensor positioned behind the second window.

16. A method of determining physiological information of a user, the method comprising:

at a device having:

a first window;

a first light sensor positioned behind the first window;

a second window;

a second light sensor positioned behind the second window;

18

a third window;

a first emitter positioned behind and off-center with respect to the third window;

a second emitter positioned behind the third window; and a first Fresnel lens positioned between the first emitter and the third window and comprising:

a first zone that is positioned above the first emitter and configured to collimate light emitted by the first emitter; and

a second zone that is positioned above the second emitter and includes ridges that act to obscure components underlying the second zone:

emitting first light from the first emitter;

receiving a first portion of the emitted first light by the first light sensor, wherein the first light sensor is located a first separation distance from the first emitter;

receiving a second portion of the emitted first light by the second light sensor, wherein:

the second light sensor is located a second separation distance from the first emitter; and

the first separation distance is less than the second separation distance; and

determining the physiological information using the received first portion of the emitted first light and the received second portion of the emitted first light.

17. The method of claim 16 comprising:

emitting second light from the second emitter;

receiving a first portion of the emitted second light by the second light sensor, and

receiving a second portion of the emitted second light by the first light sensor,

wherein determining the physiological information comprises determining the physiological information using the received first portion of the emitted second light and the received second portion of the emitted second light.

18. The method of claim 17, comprising:

generating first signals from the received first portion of the emitted first light and the received first portion of the emitted second light;

generating second signals from the received second portion of the emitted first light and the received second portion of the emitted second light; and

selecting between the first signals and the second signals based on the user's skin type.

19. The method of claim 17, further comprising:

generating first signals from the received first portion of the emitted first light and the received first portion of the emitted second light;

generating second signals from the received second portion of the emitted first light and the received second portion of the emitted second light; and

selecting between the first signals and the second signals based on a usage condition.

20. The method of claim 16, wherein the first emitter and the second emitter have different emission wavelengths.

\* \* \* \* \*