

US 20050247870A9

(19) **United States**
(12) **Patent Application Publication**
Park

(10) **Pub. No.: US 2005/0247870 A9**
(48) **Pub. Date: Nov. 10, 2005**
CORRECTED PUBLICATION

(54) **METHOD AND APPARATUS FOR AN ELECTROSPRAY NEEDLE FOR USE IN MASS SPECTROMETRY**

Related U.S. Application Data

(76) Inventor: **Melvin A. Park**, Billerica, MA (US)

(63) Continuation of application No. 09/639,531, filed on Aug. 16, 2000, now Pat. No. 6,525,313.

Correspondence Address:
WARD & OLIVO
708 Third Avenue
New York, NY 10017 (US)

Publication Classification

(51) **Int. Cl.⁷** **H01J 49/00; B01D 59/44**
(52) **U.S. Cl.** **250/288**

(21) Appl. No.: **10/371,152**

(57) **ABSTRACT**


(22) Filed: **Feb. 21, 2003**

The present invention relates to a spray needle for use in electrospray ionization (ESI) for mass spectrometry. A spray needle is disclosed which is constructed to have an opening along its length such that a sample solution may be more readily introduced or loaded therein. Further, the design of the spray needle of the invention is more durable than the prior art spray needles and may be reusable. Because sample loading is more readily achieved, the spray needle of the invention is appropriate for use with a fully automated system for the analysis of samples.

Prior Publication Data

(15) Correction of US 2004/0011954 A1 Jan. 22, 2004
See Filing Date

(65) US 2004/0011954 A1 Jan. 22, 2004

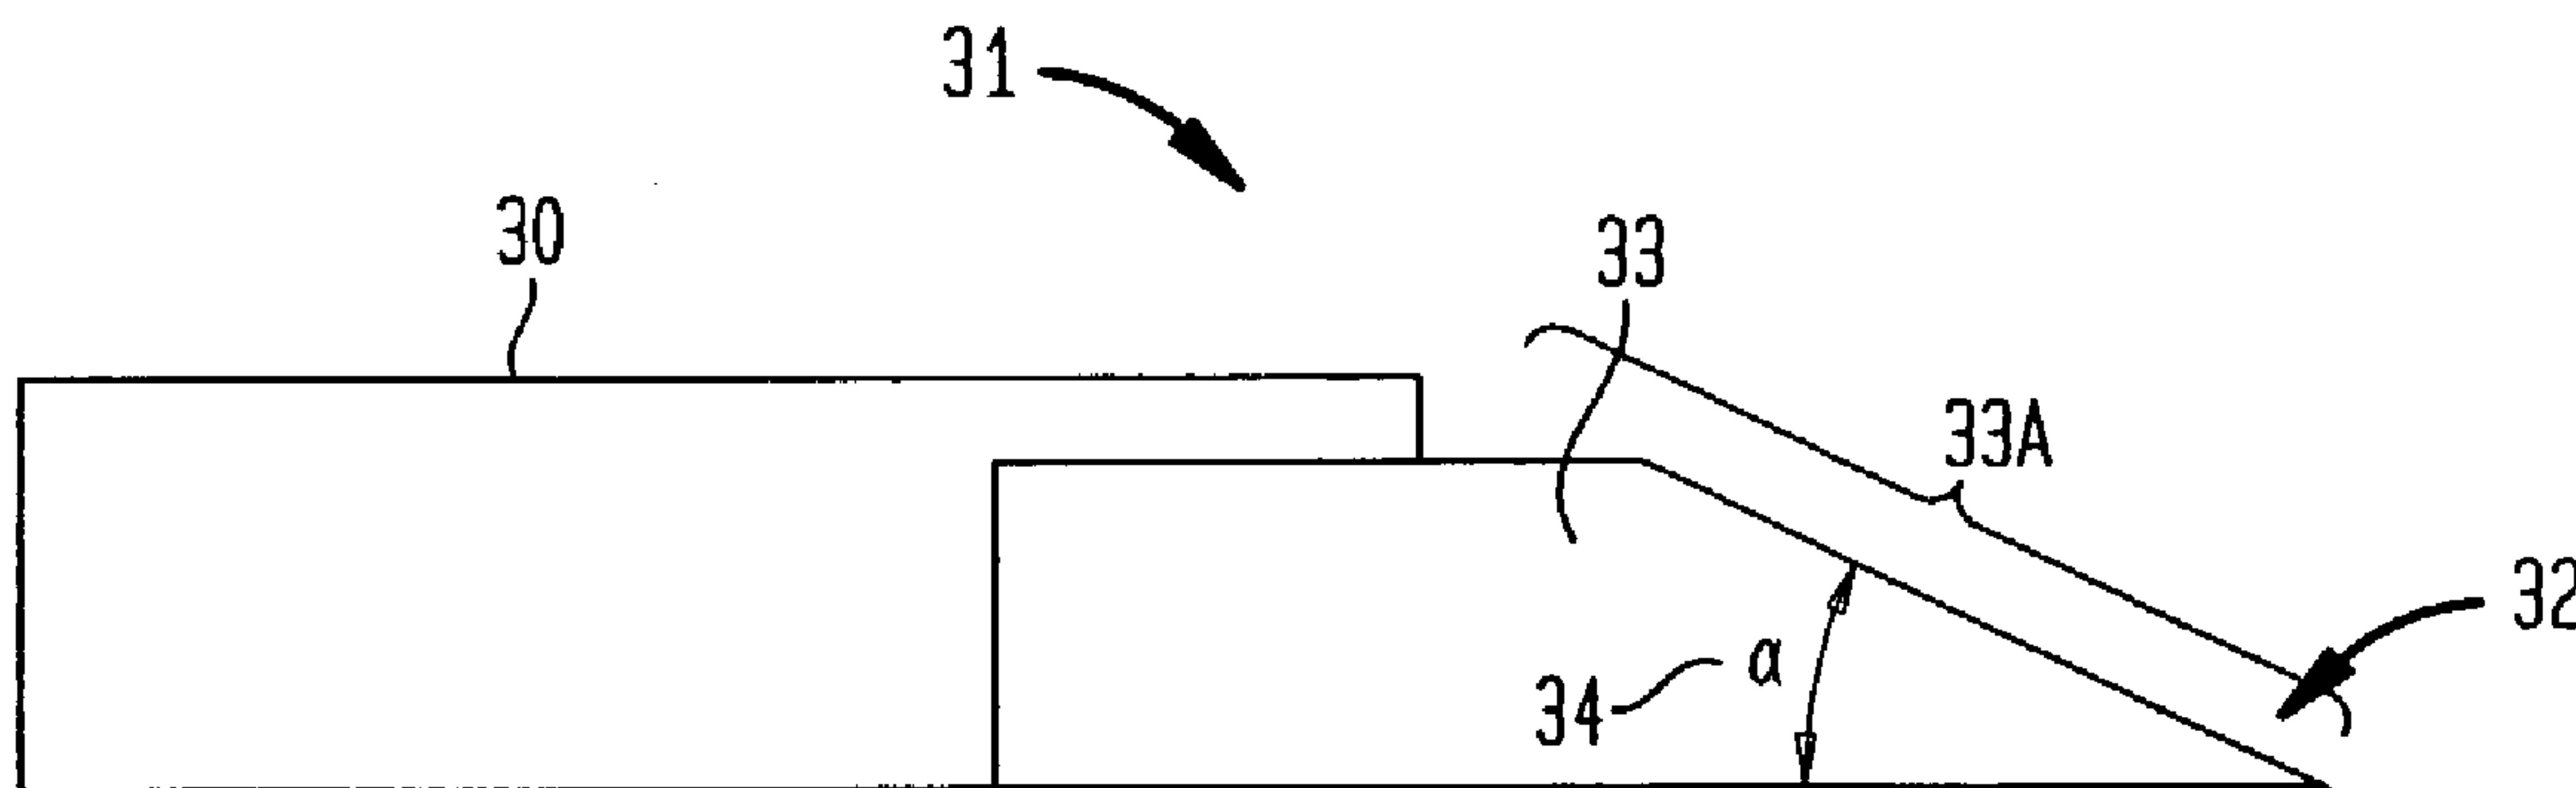

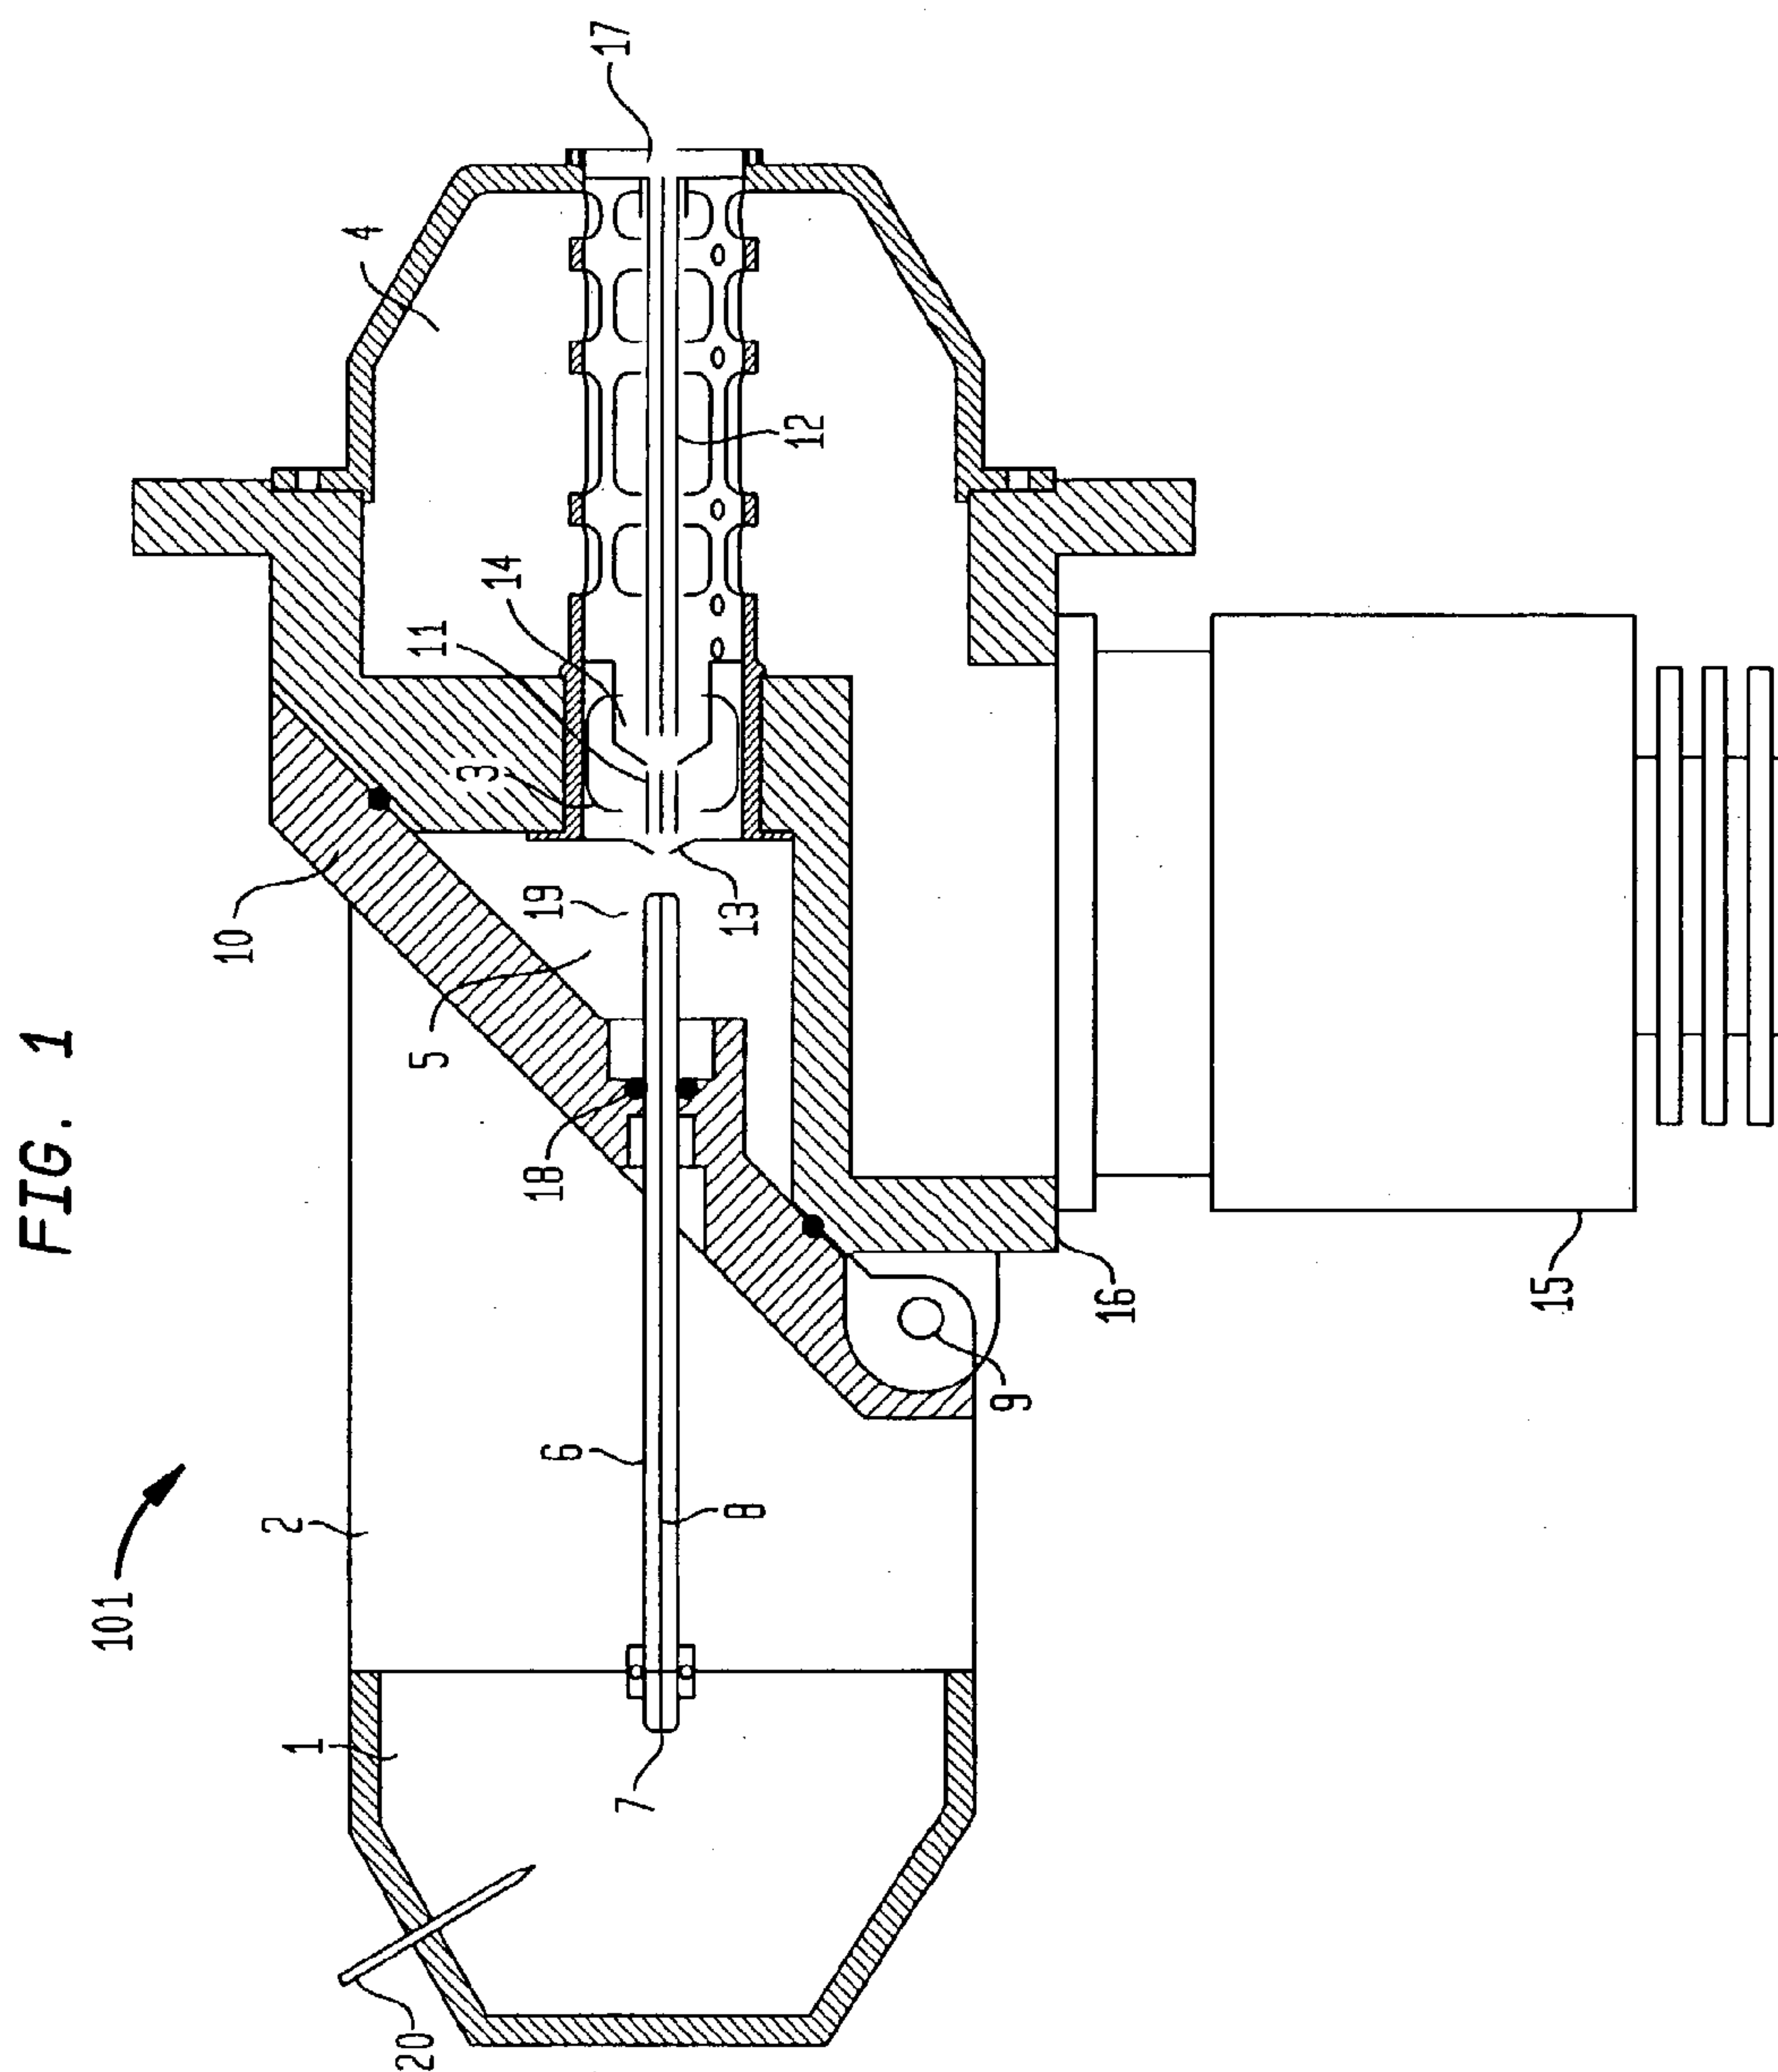


FIG. 2
(PRIOR ART)

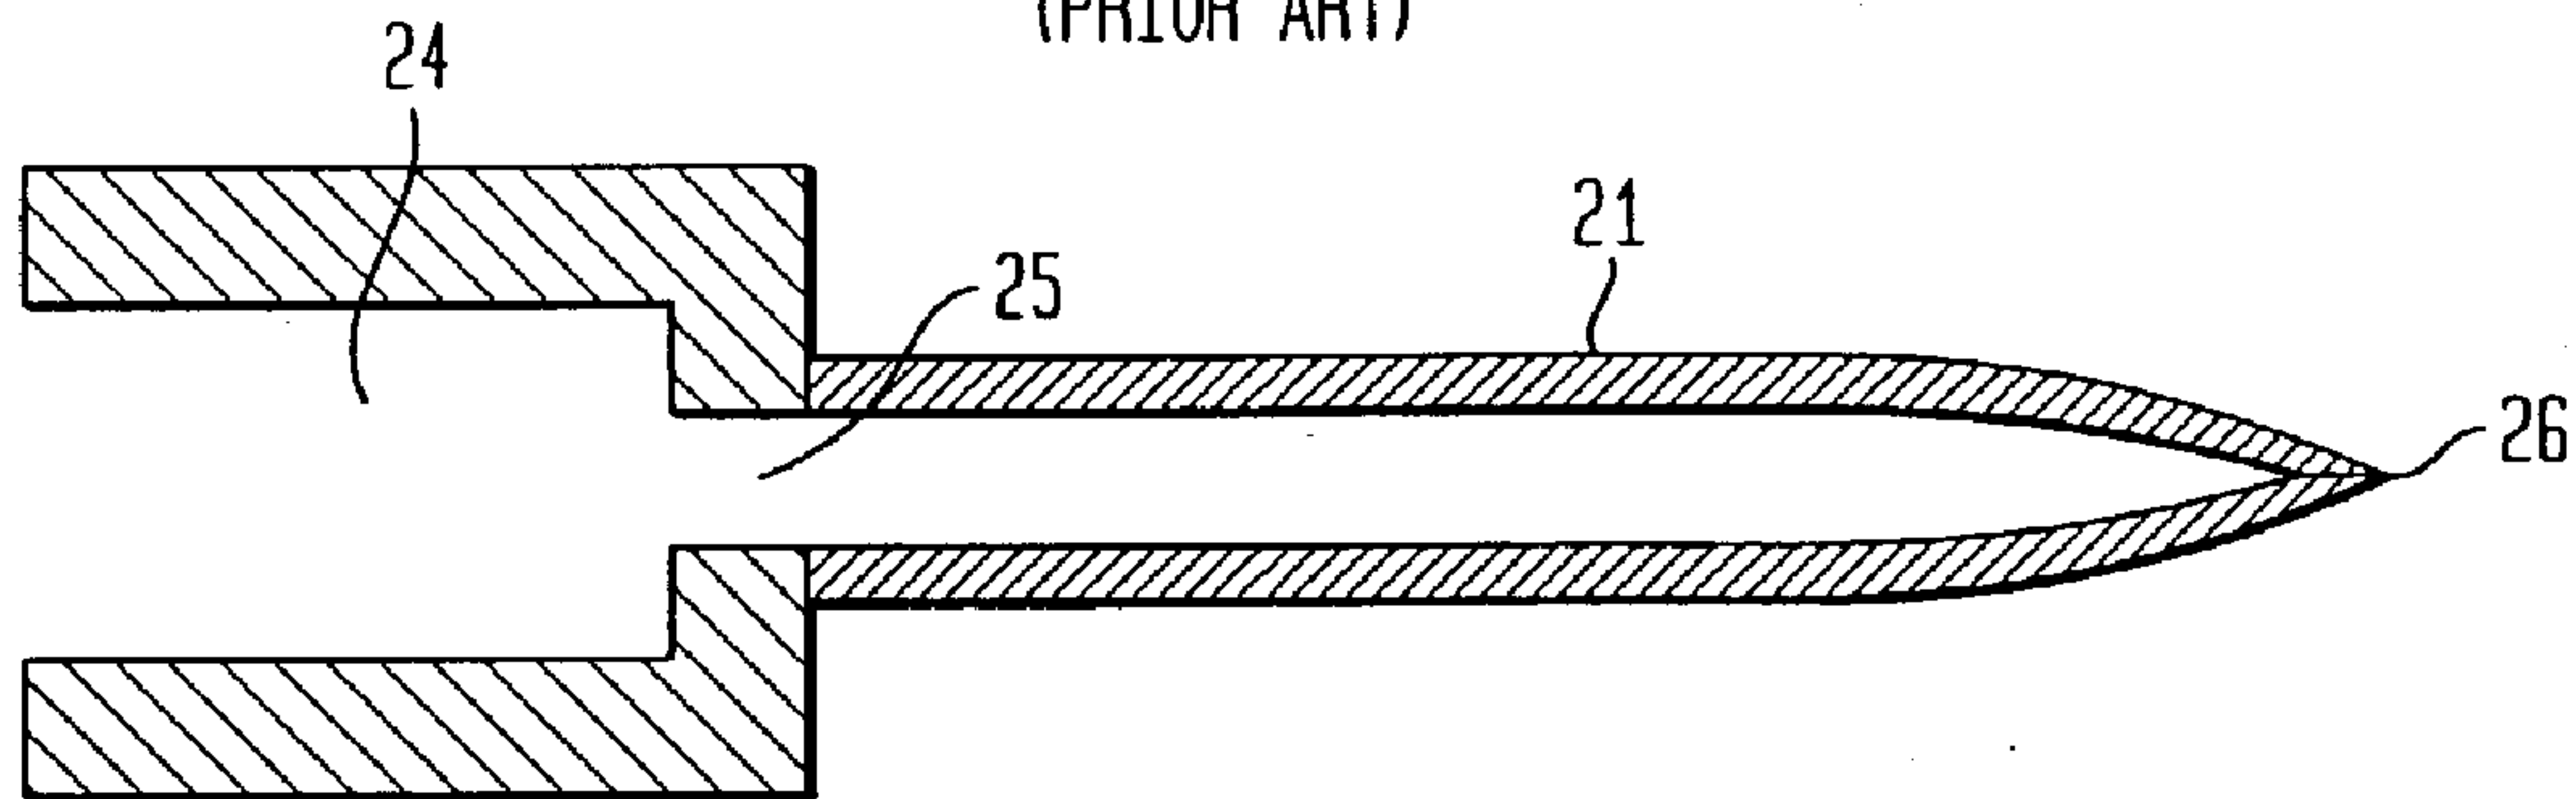


FIG. 3
(PRIOR ART)

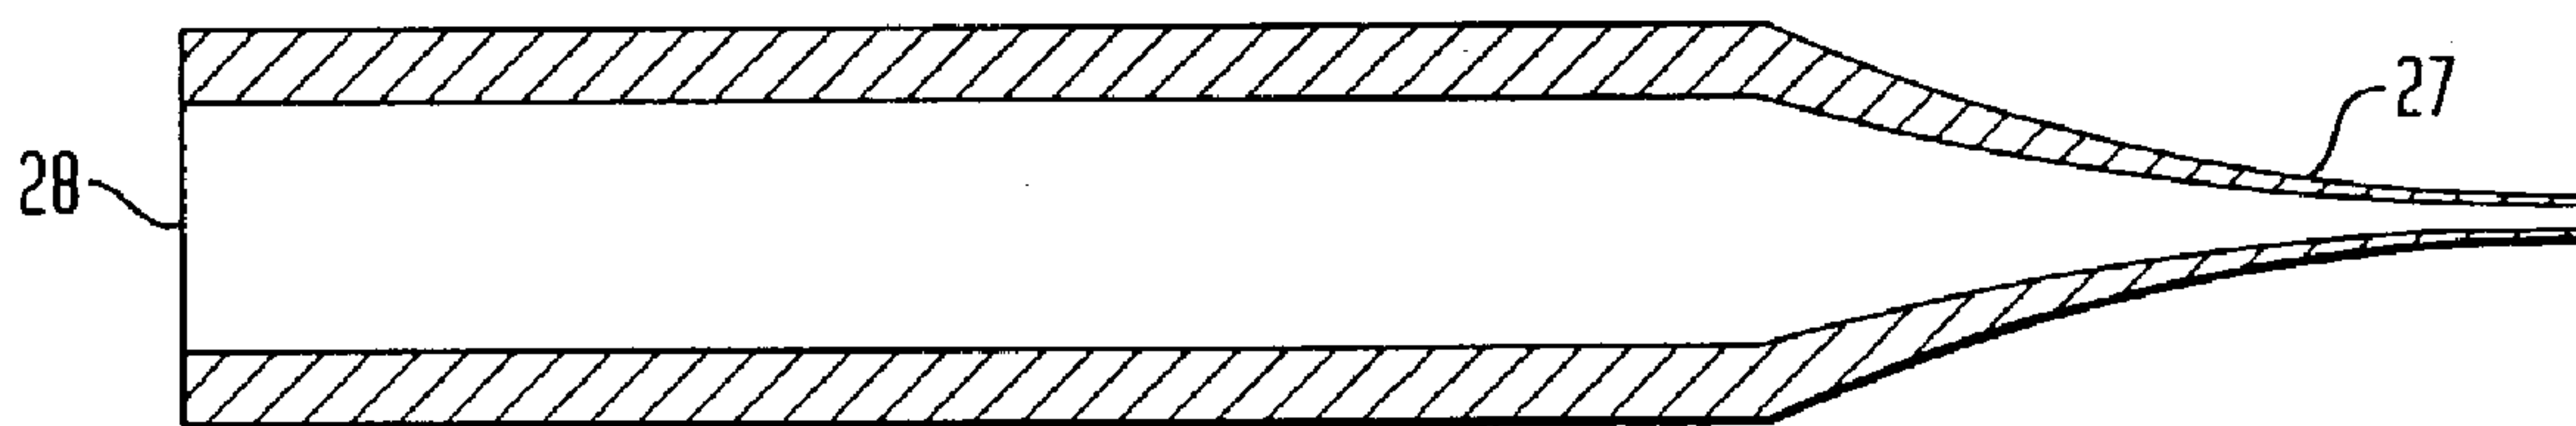


FIG. 4
(PRIOR ART)

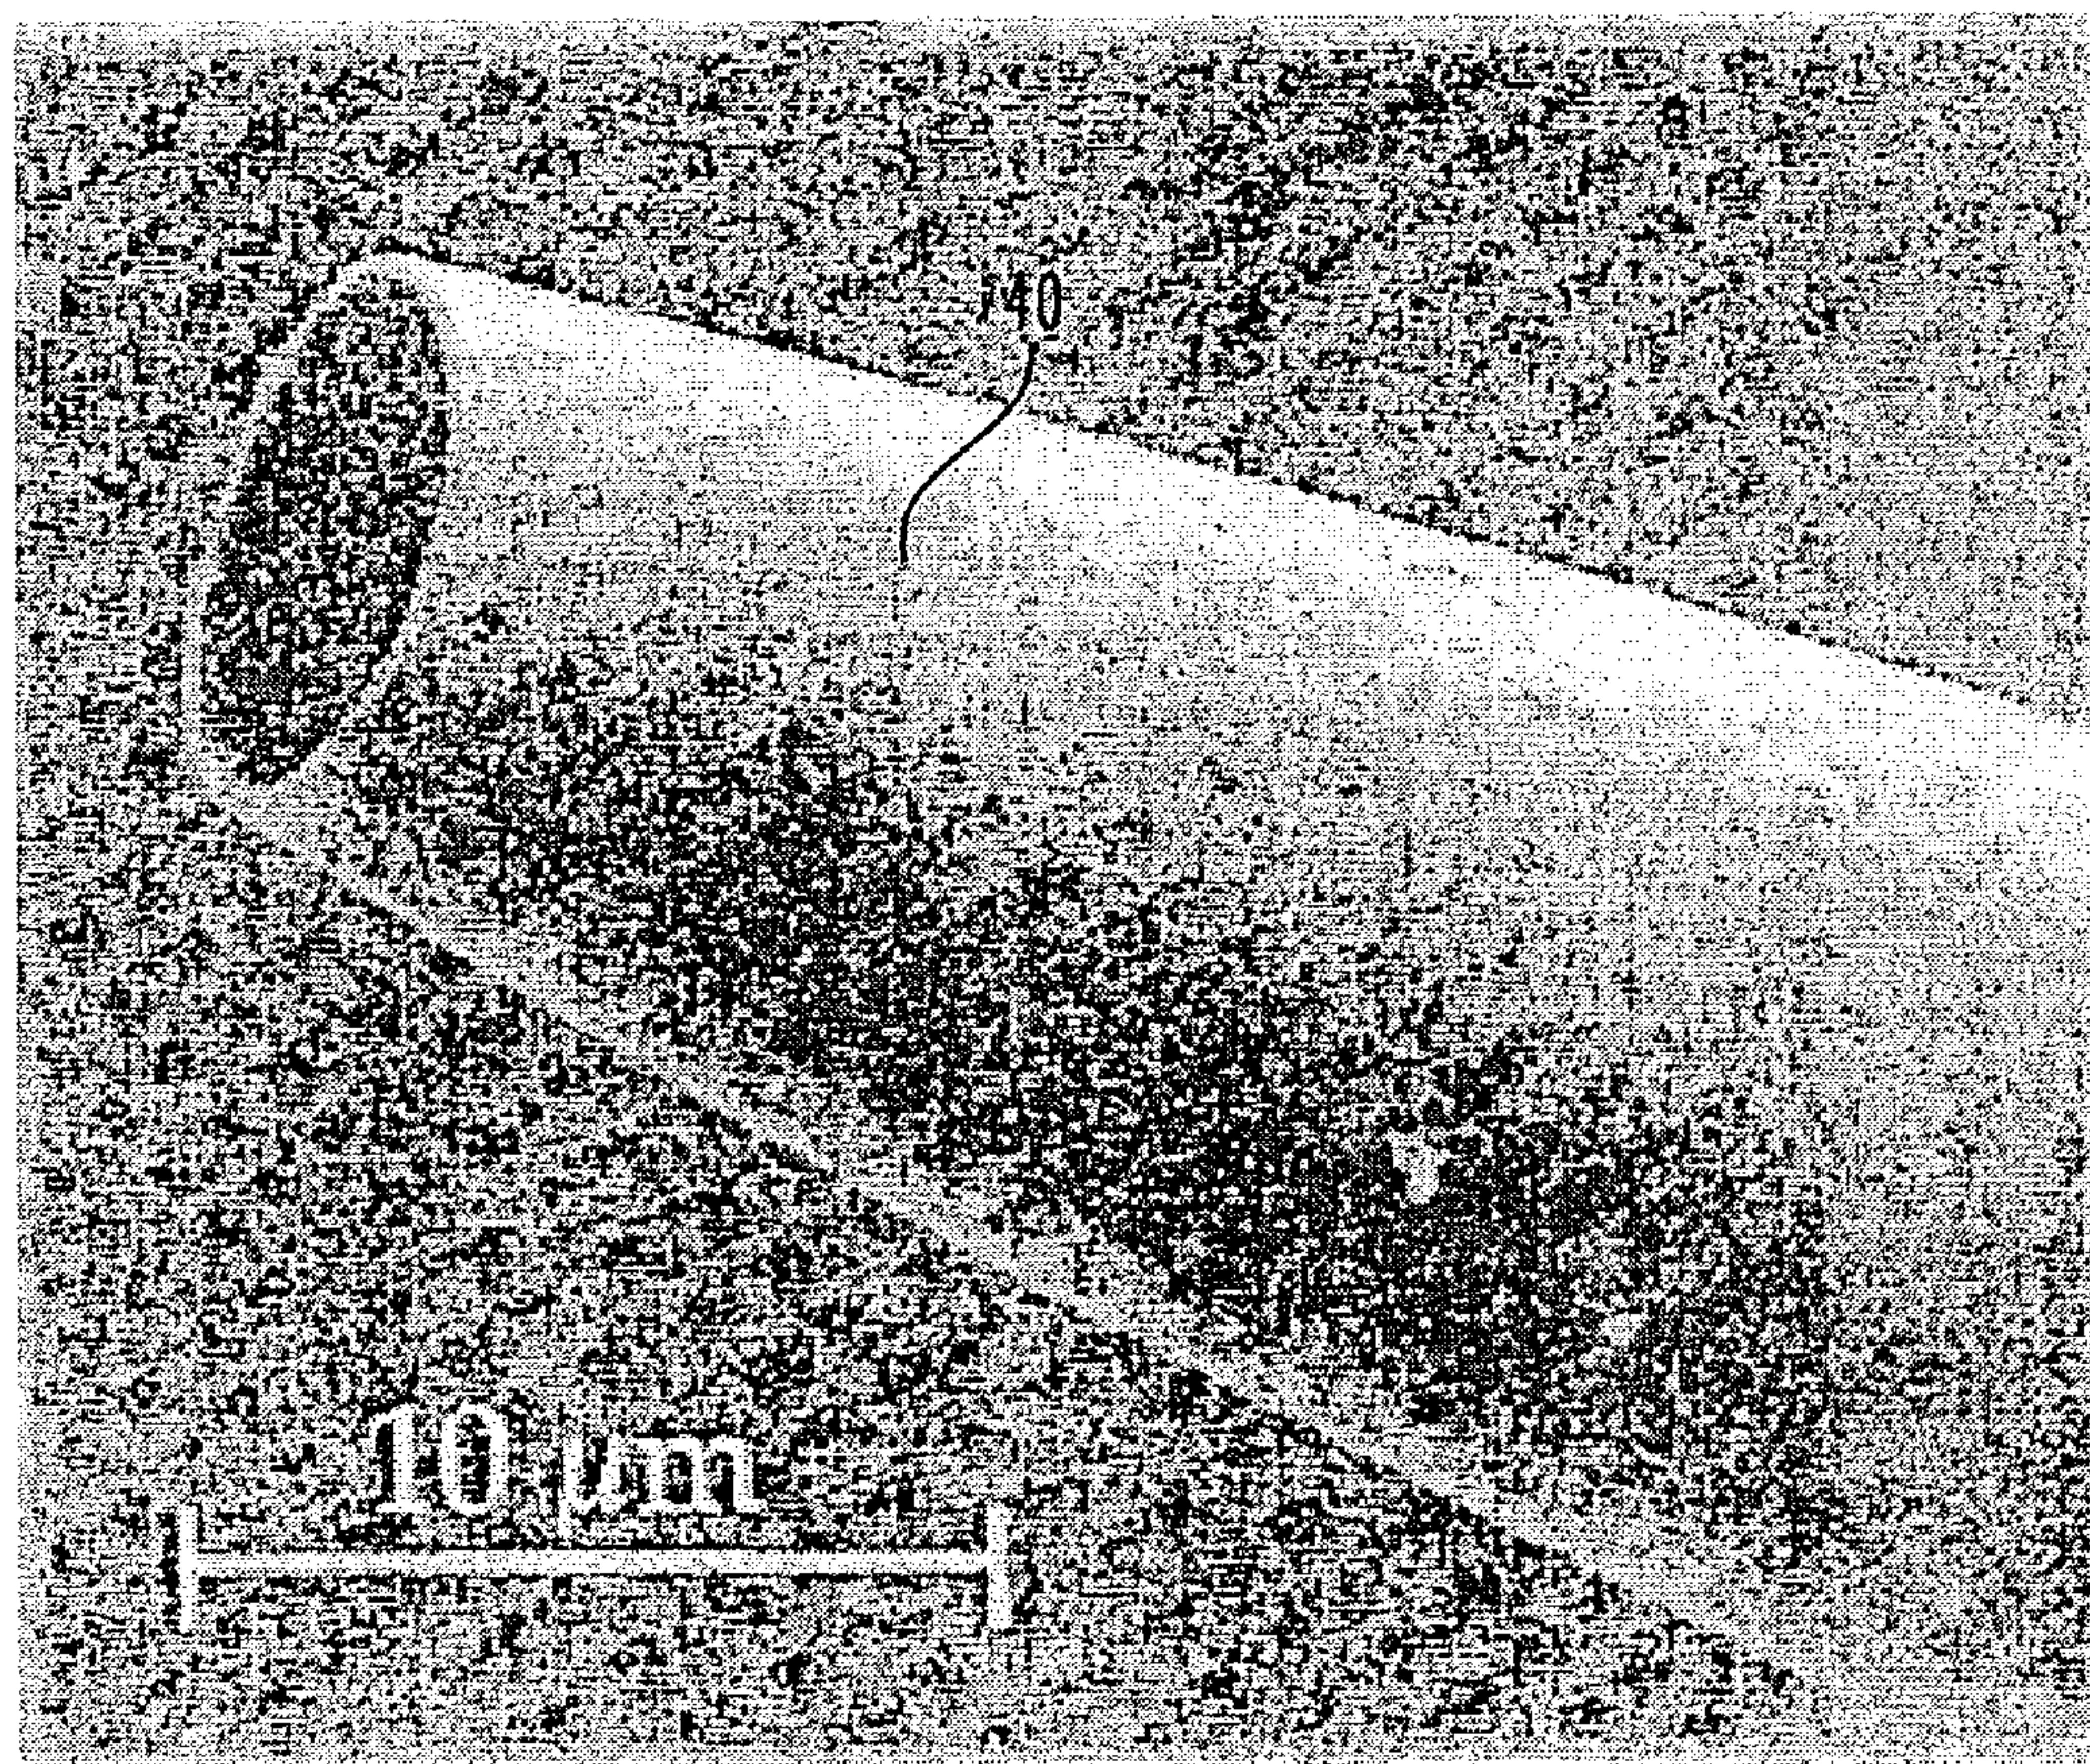


FIG. 5A

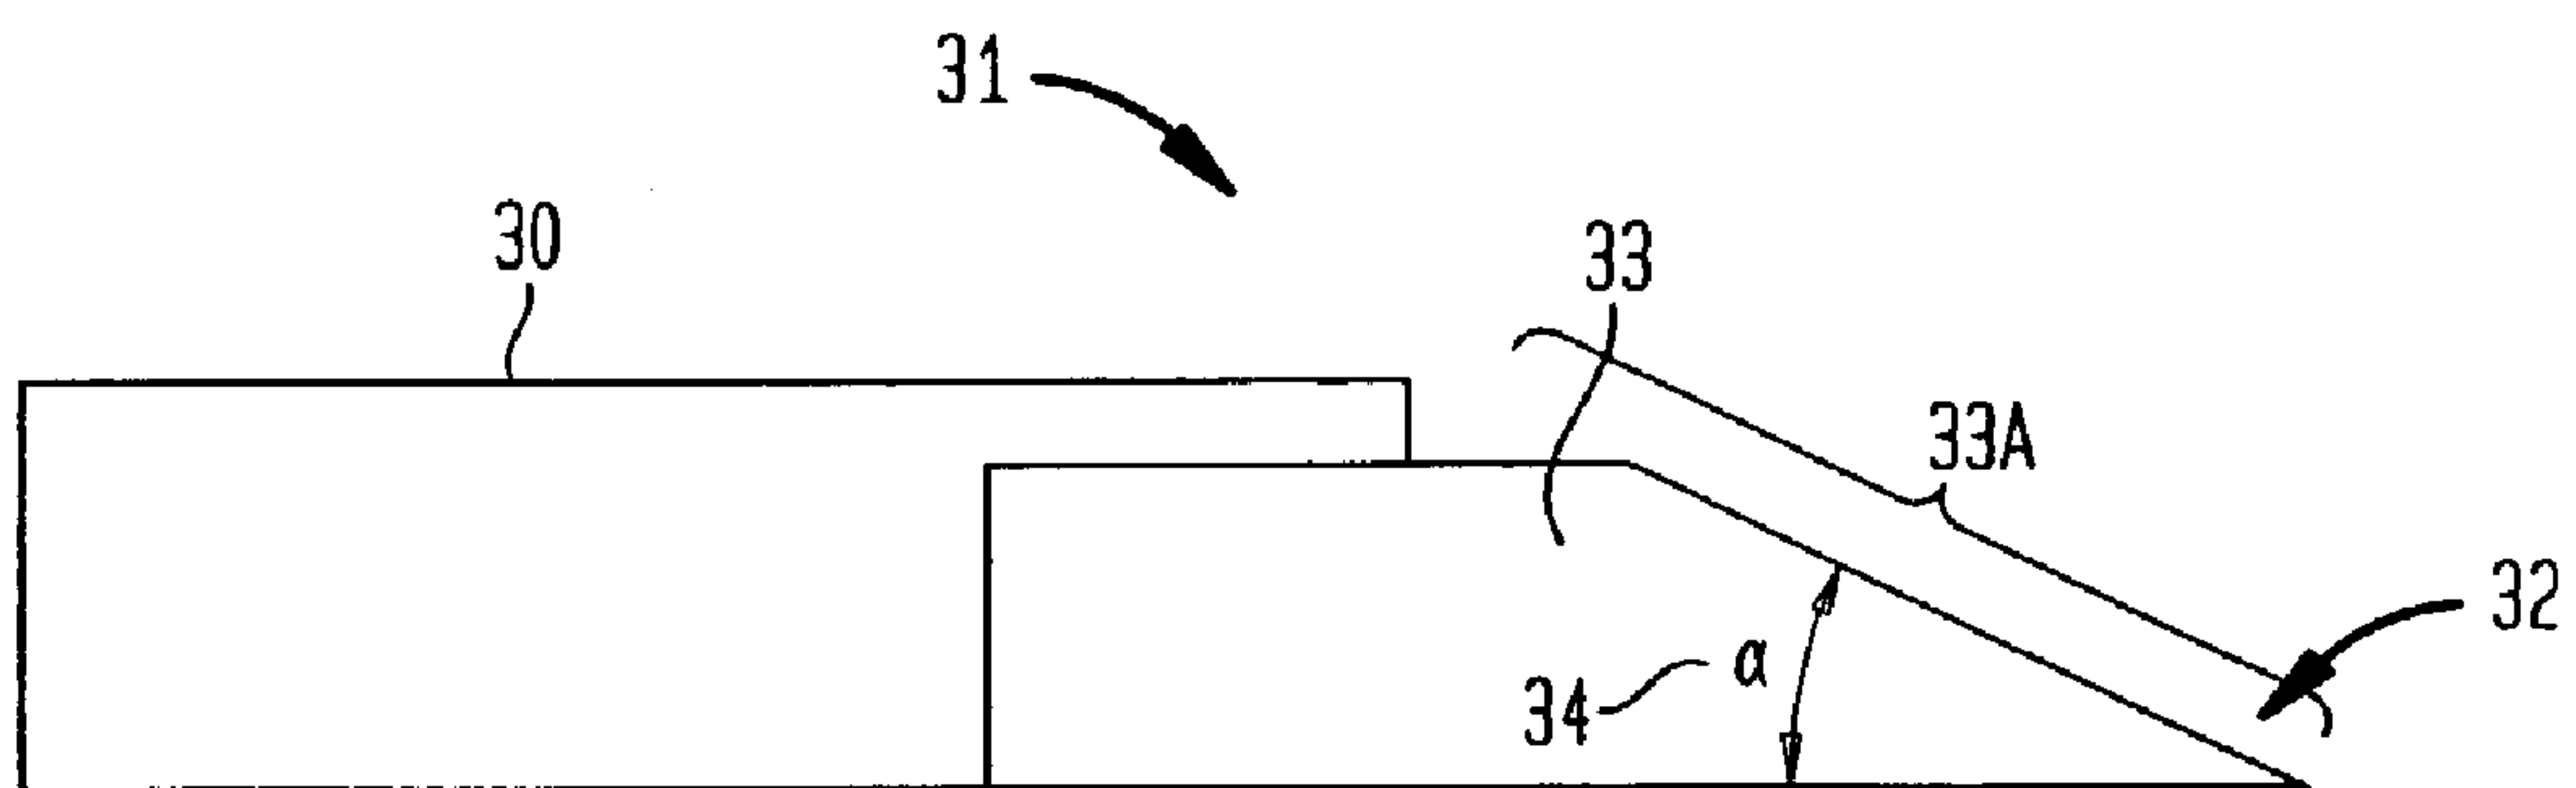


FIG. 5B

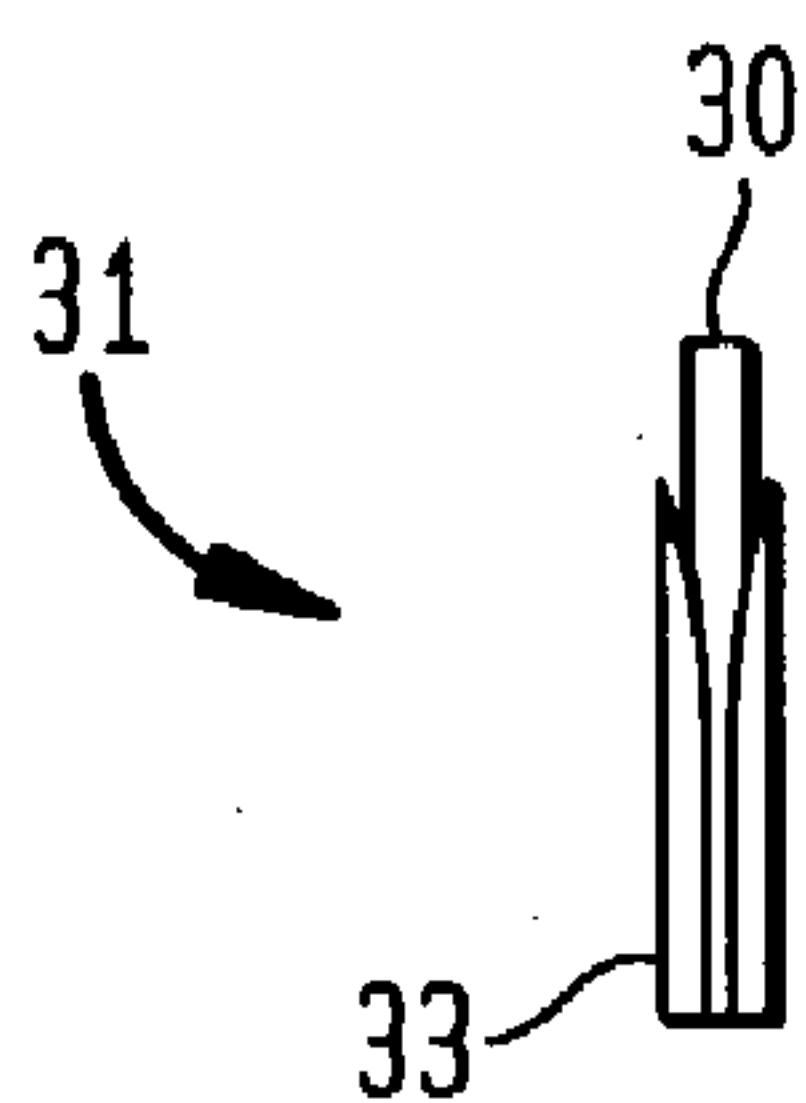


FIG. 5C

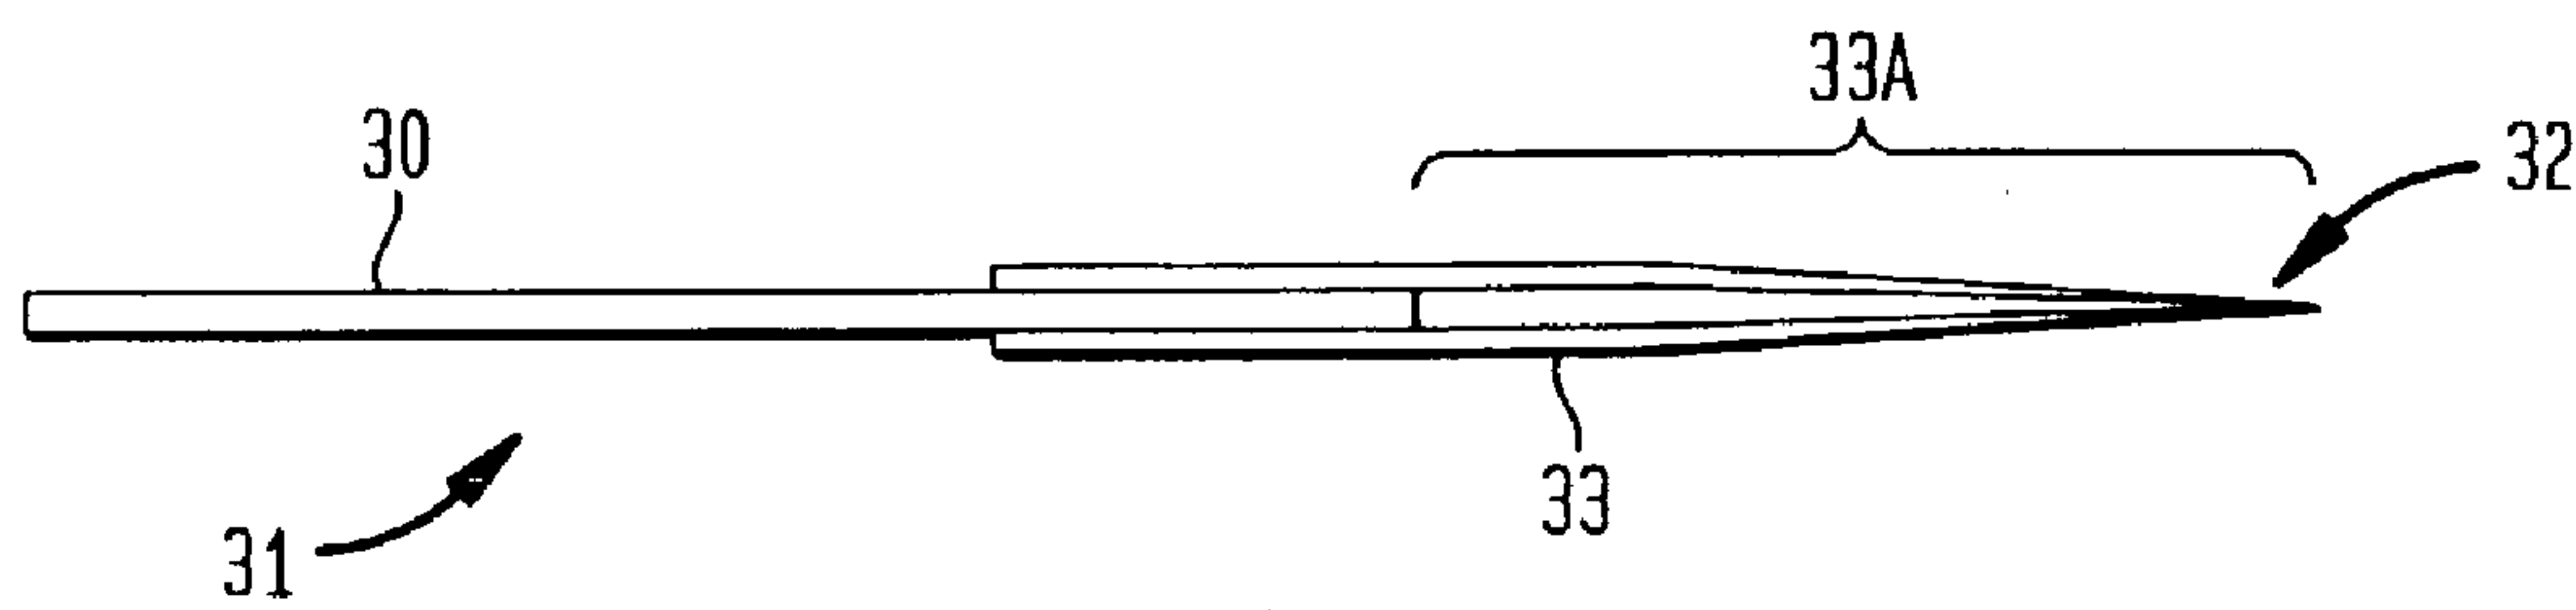


FIG. 6A

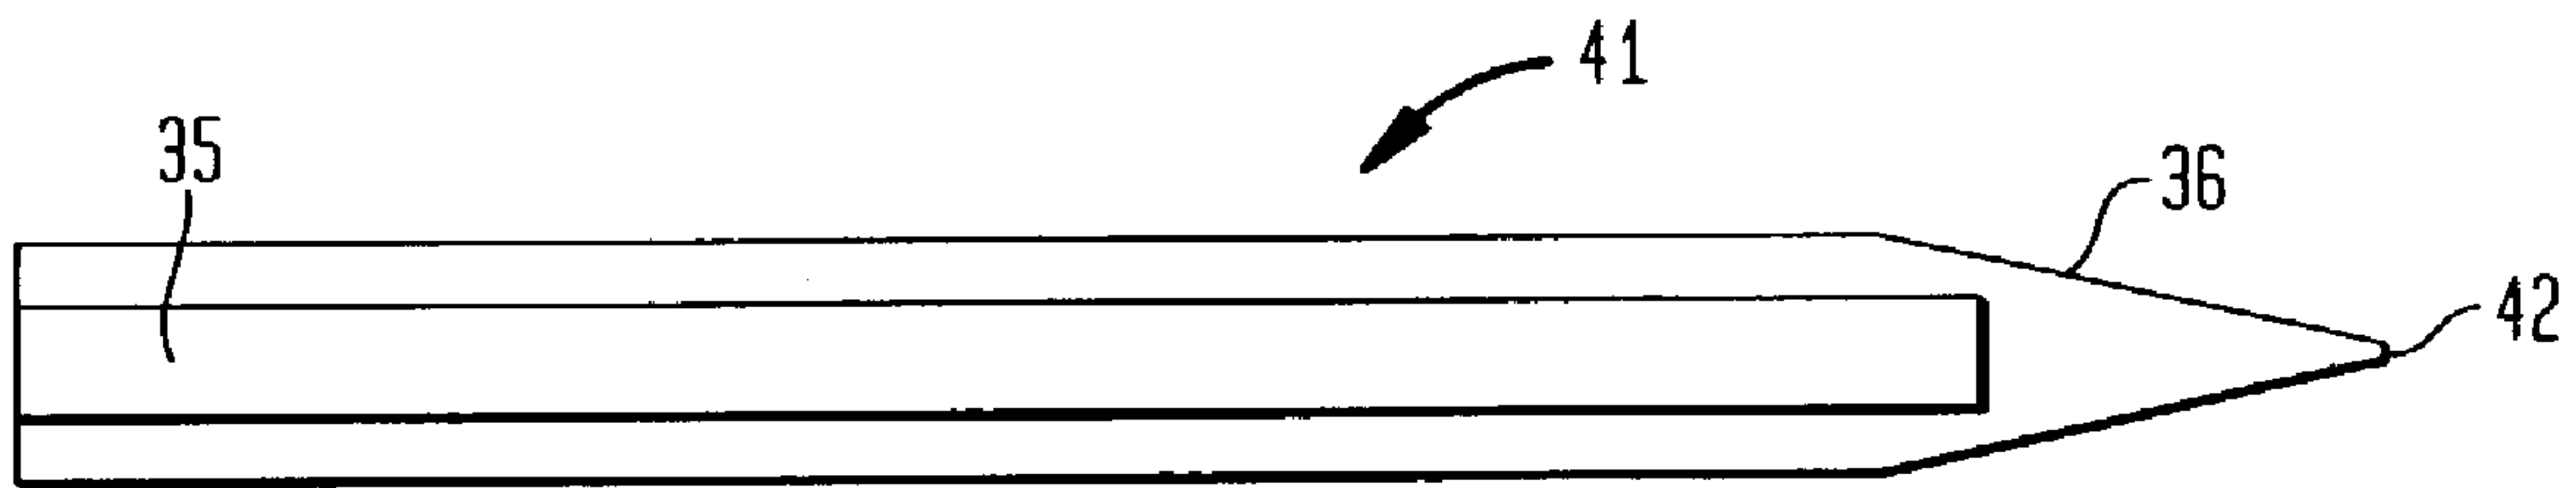


FIG. 6B

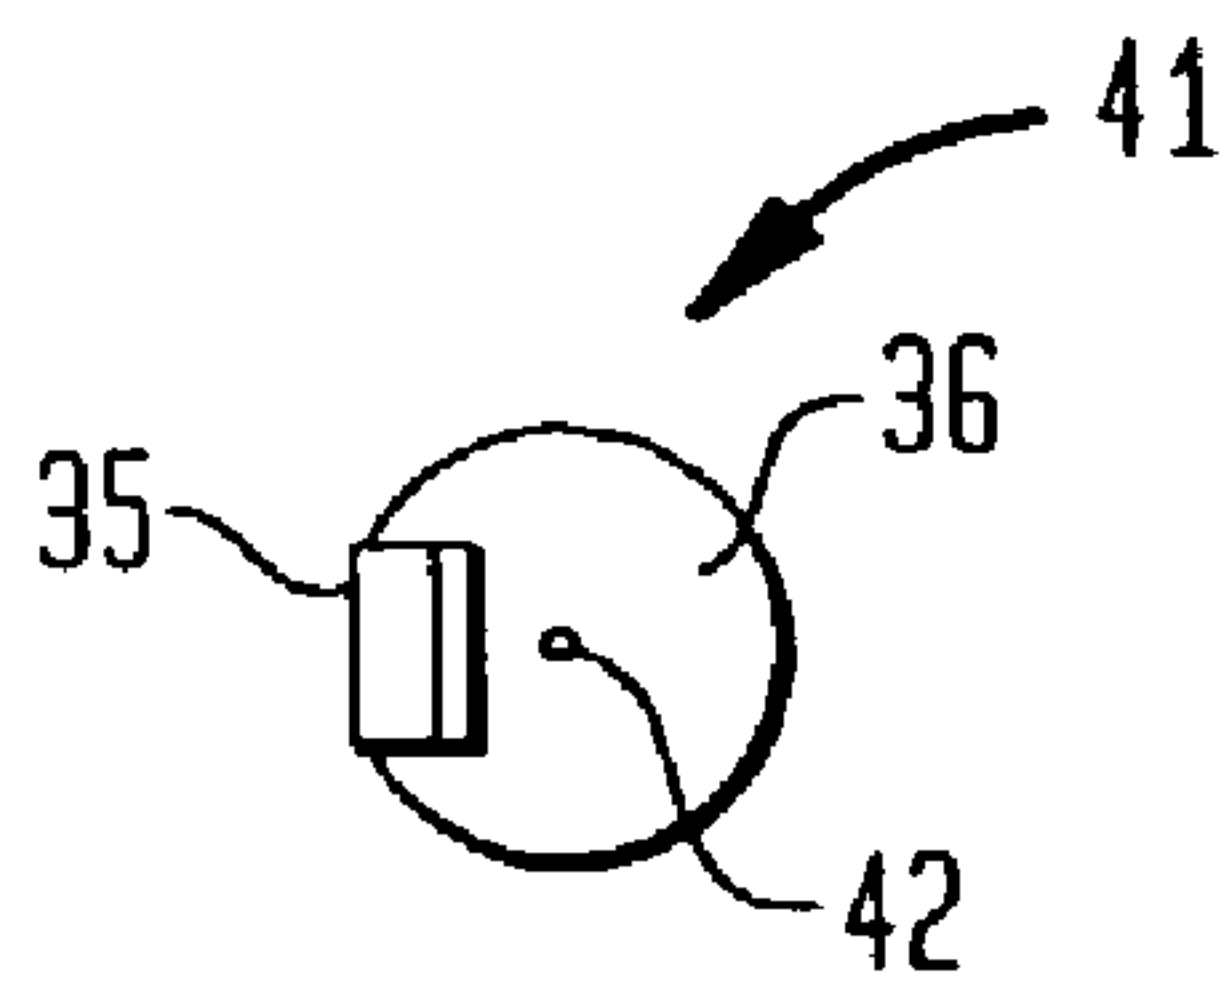


FIG. 6C

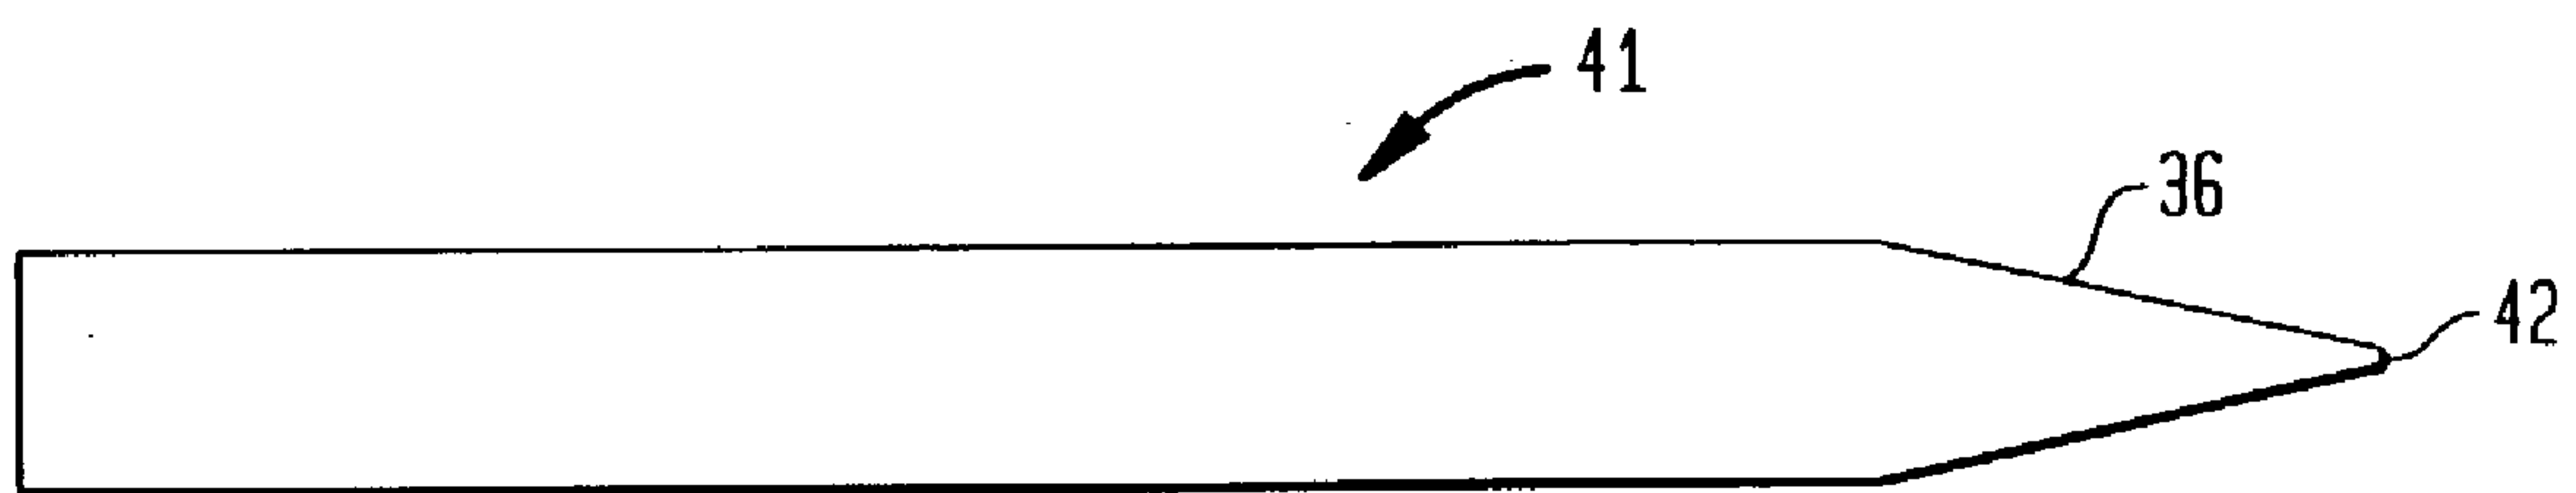


FIG. 7A

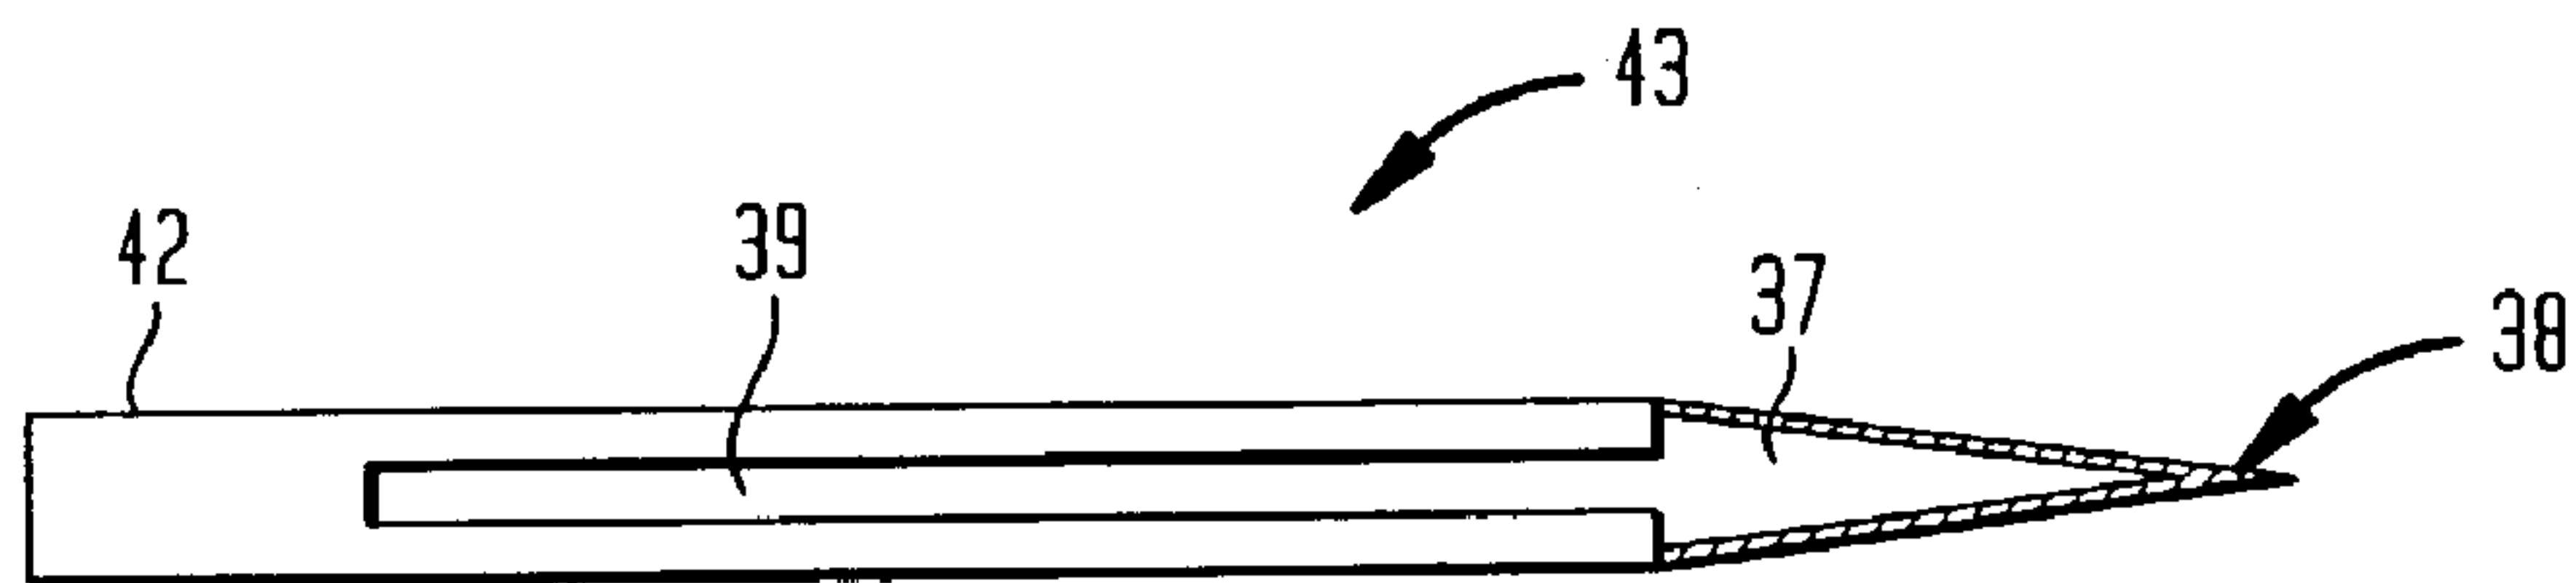


FIG. 7B

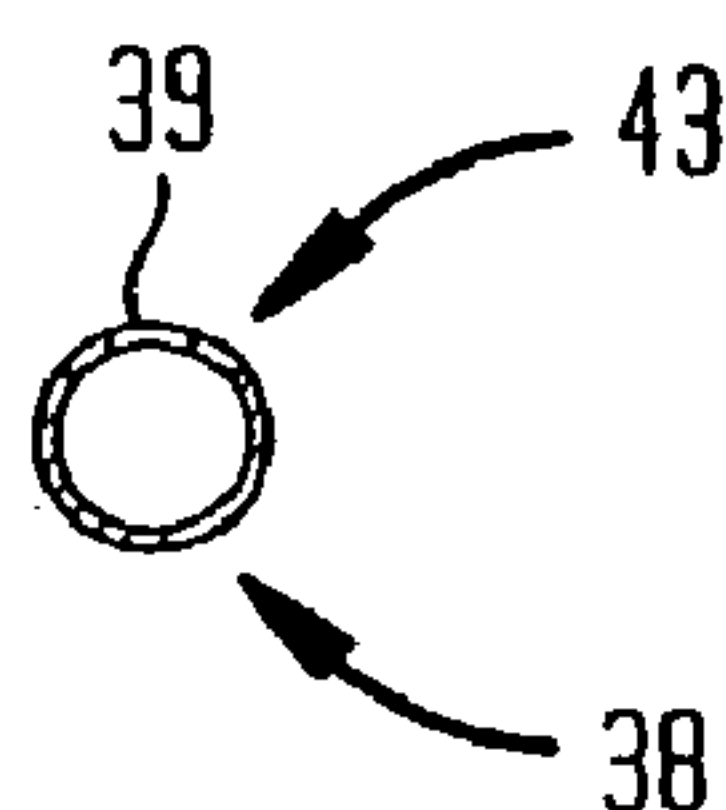


FIG. 7C

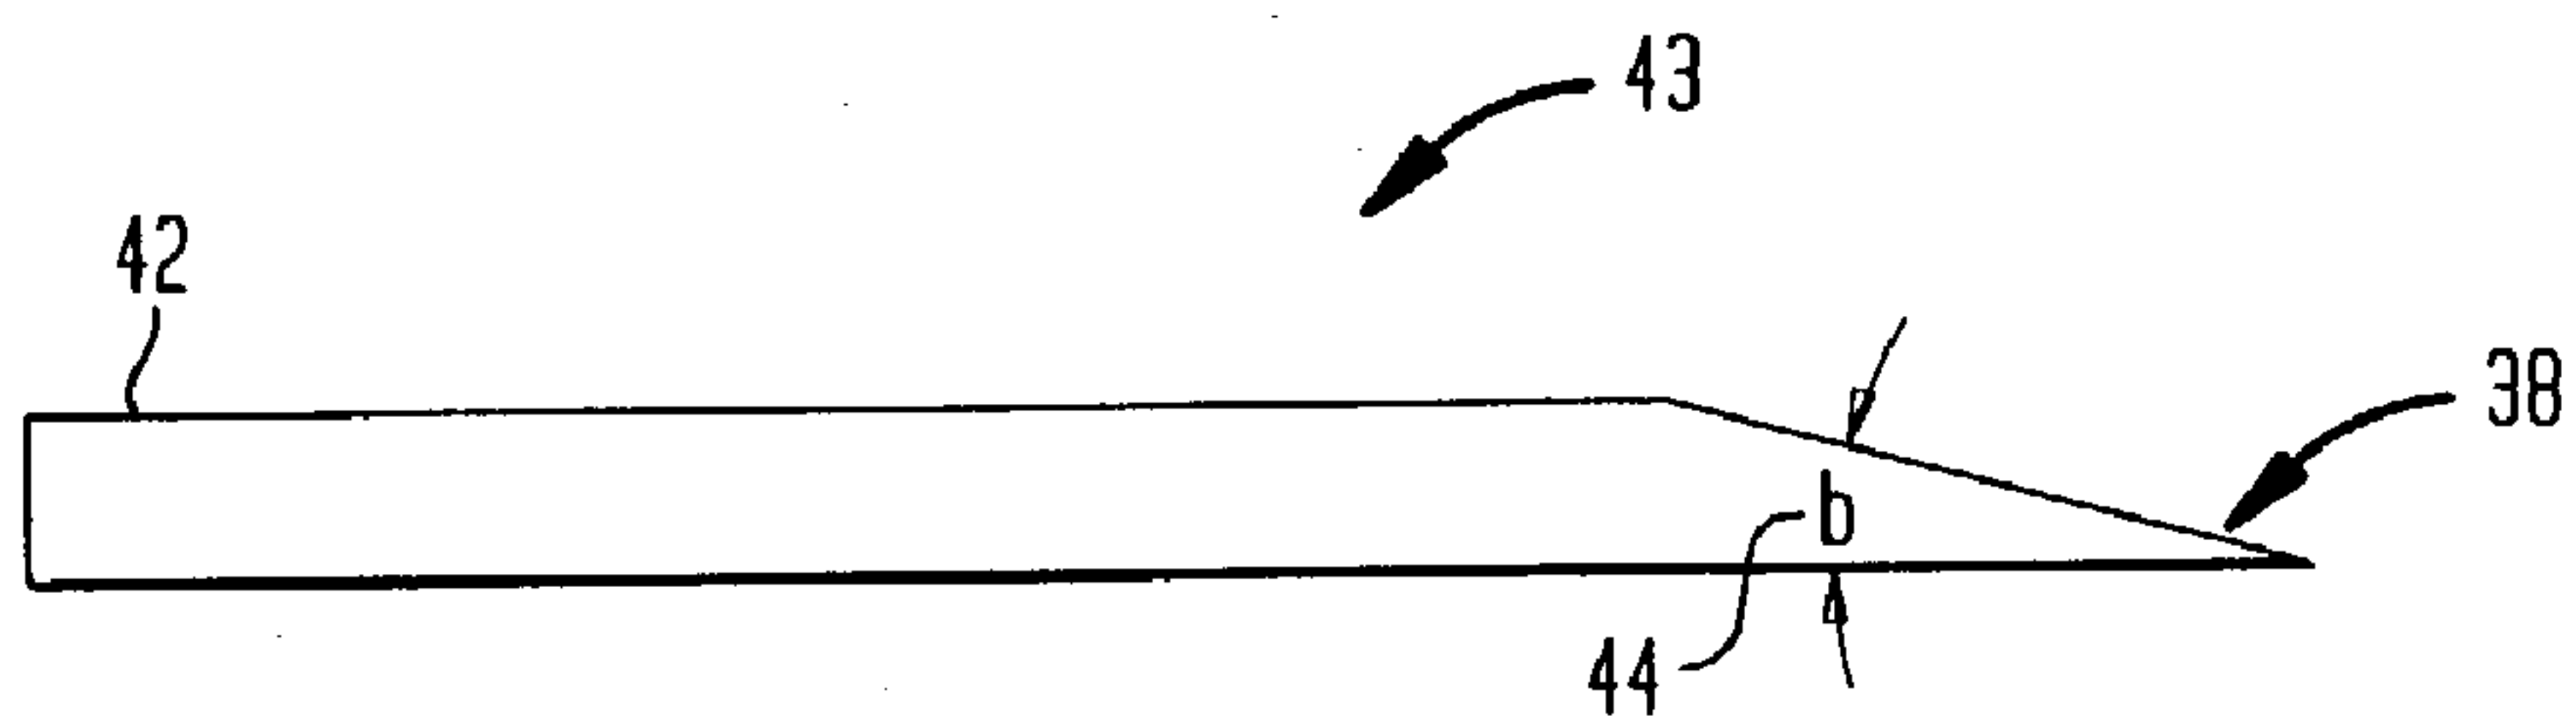


FIG. 8

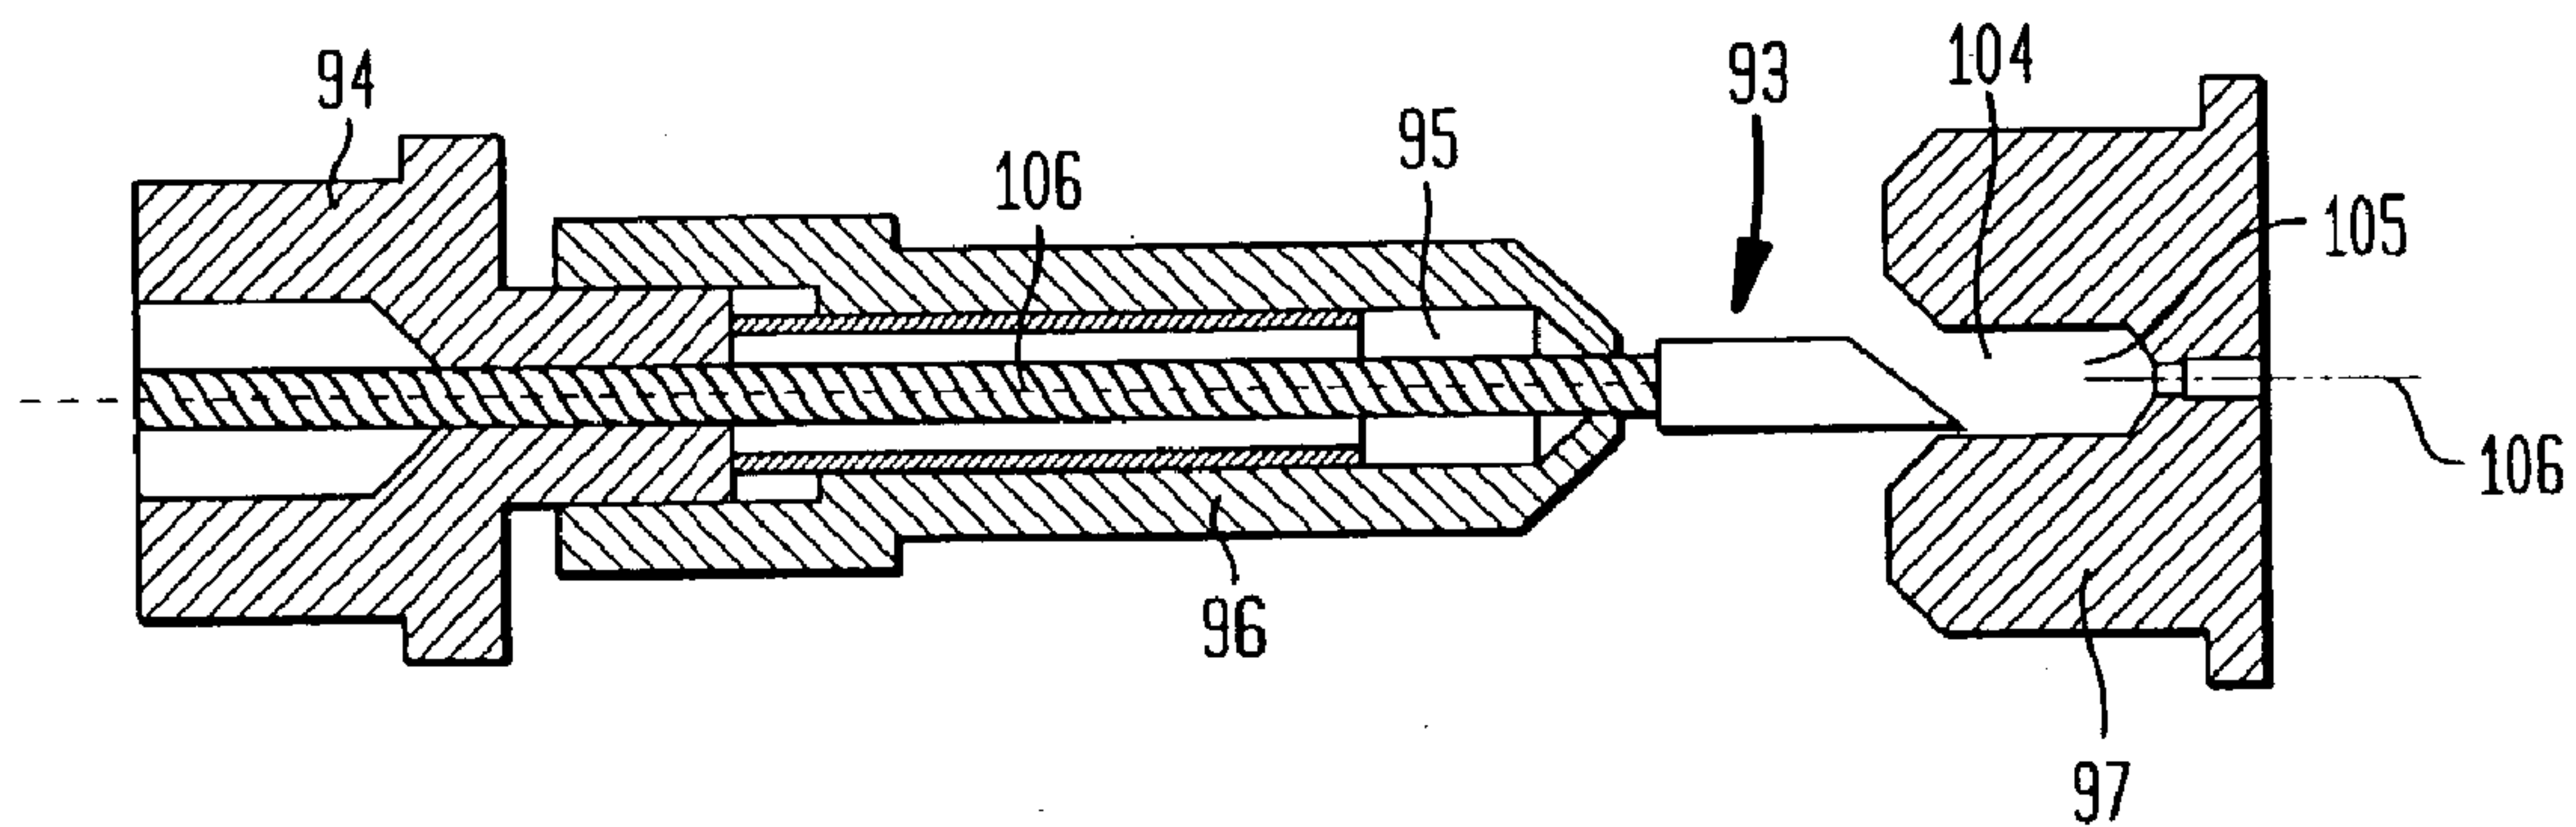


FIG. 9

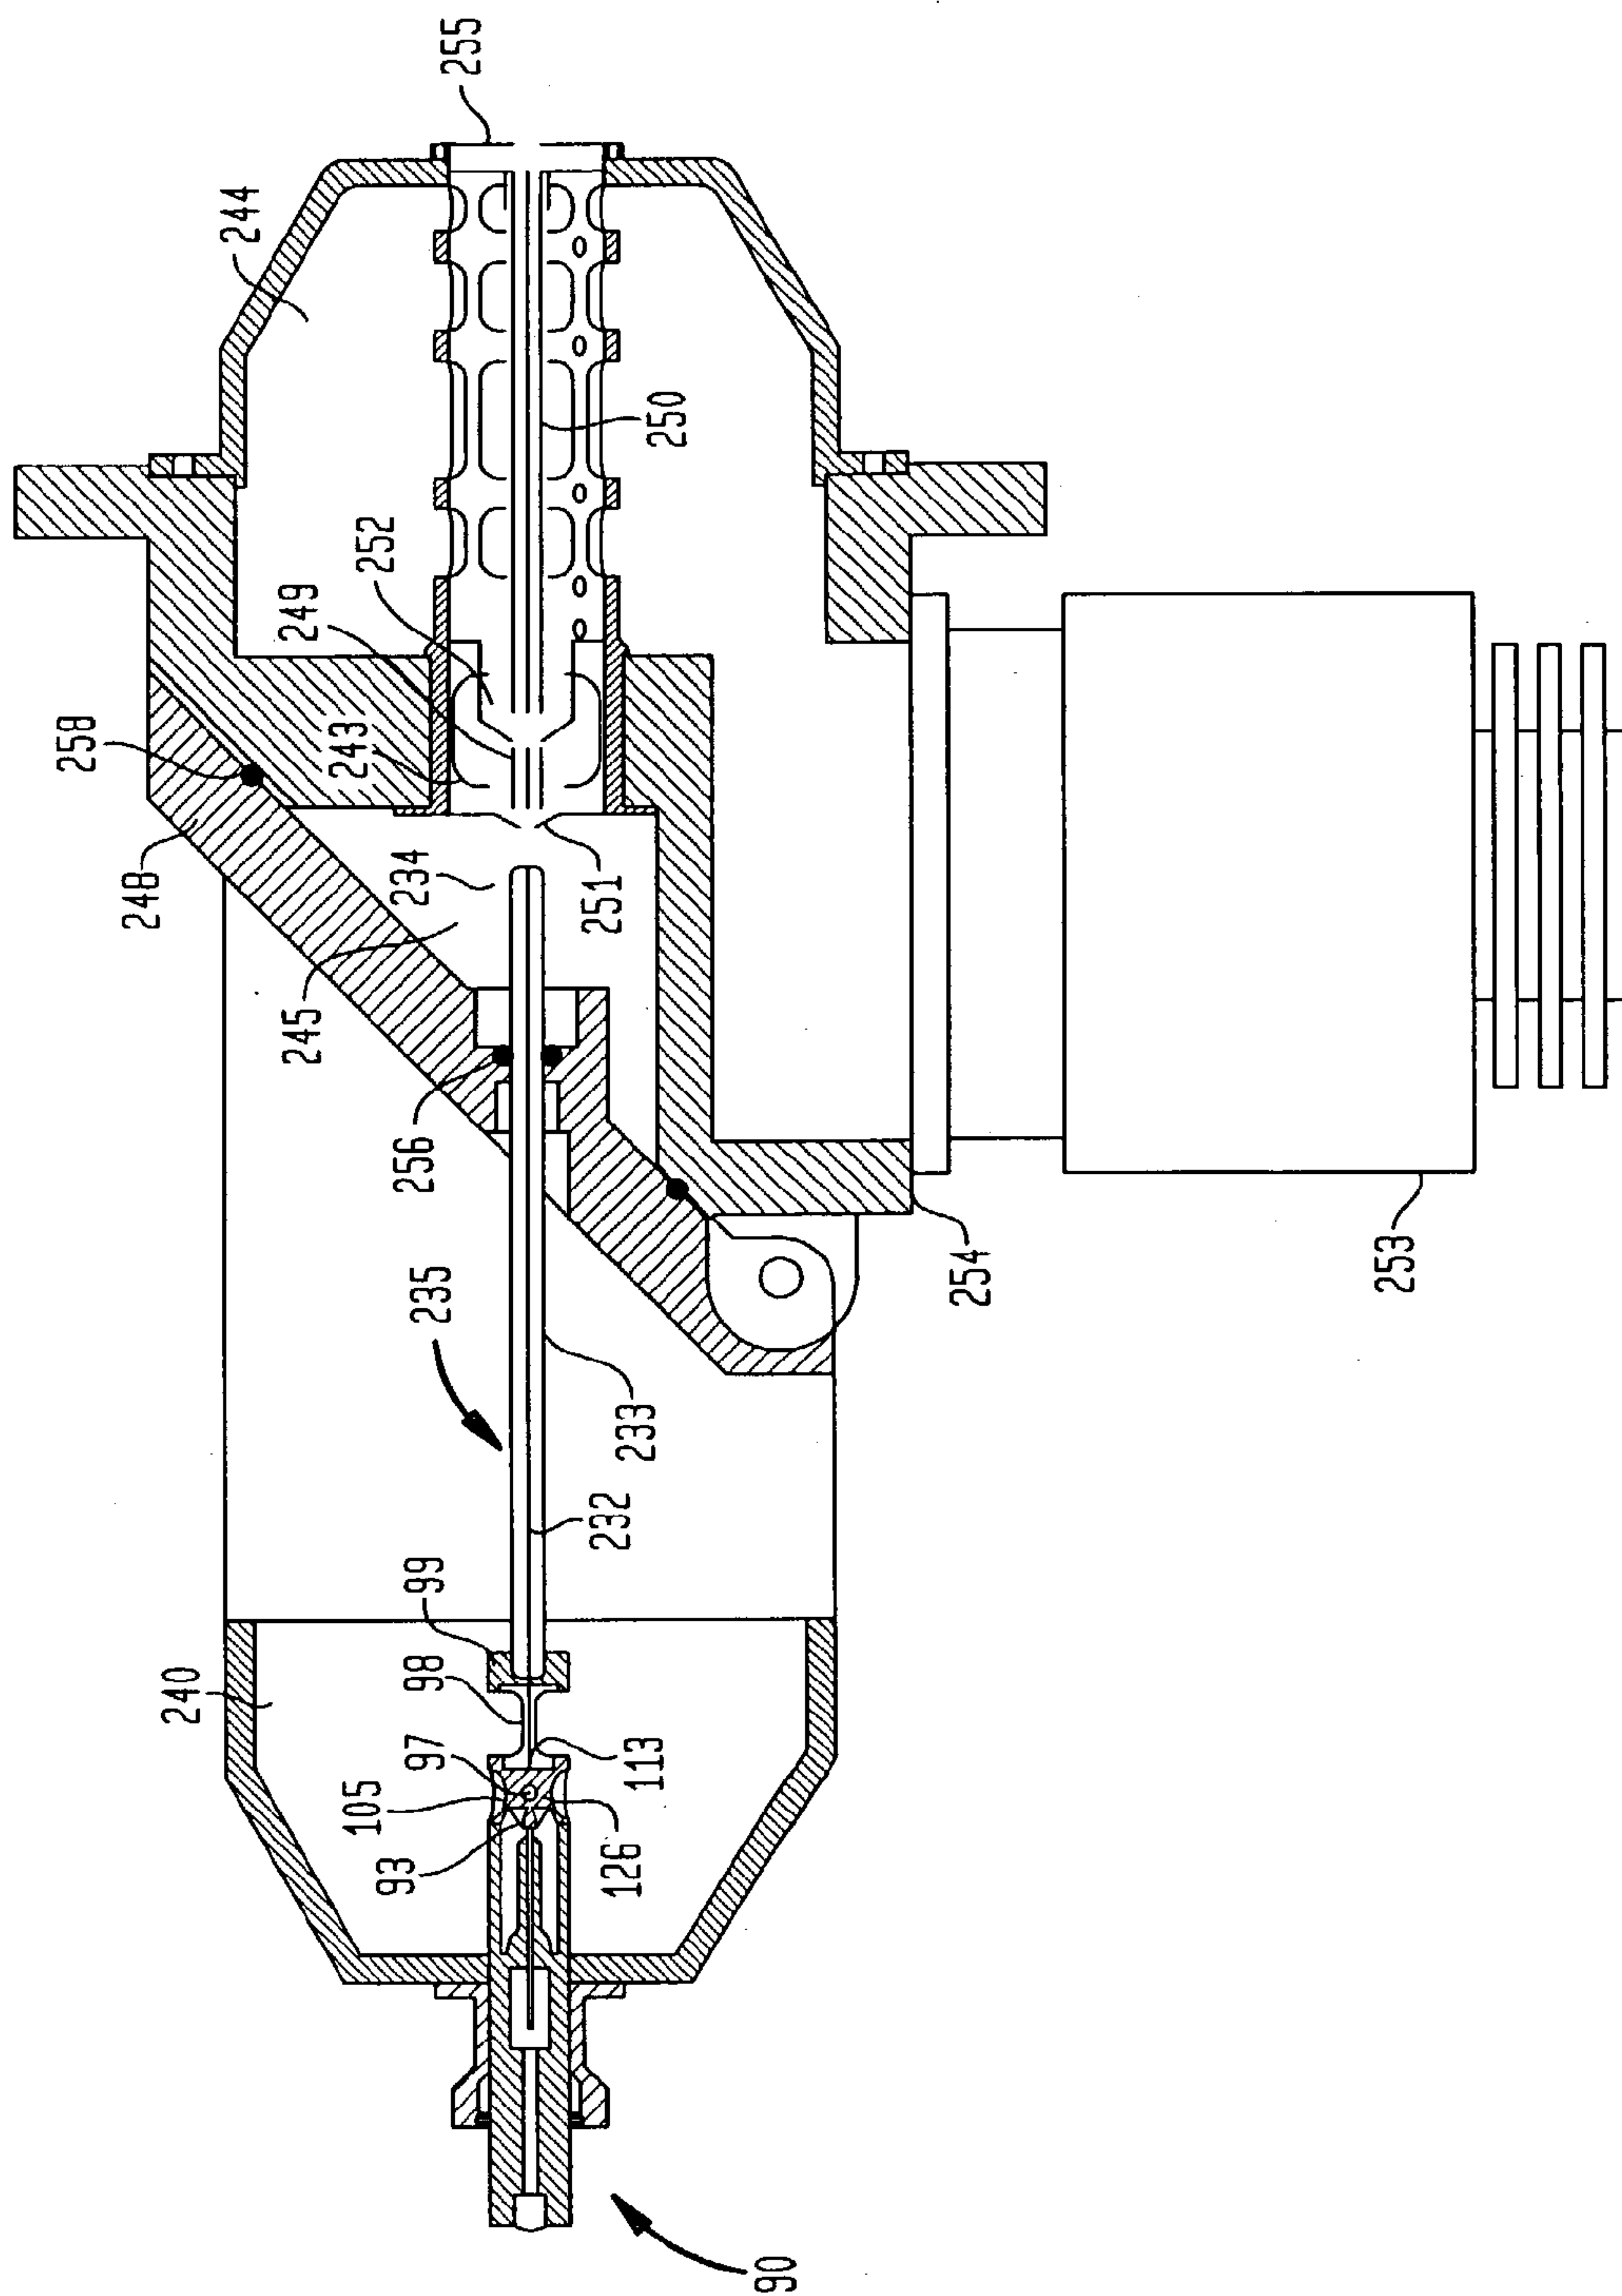


FIG. 10

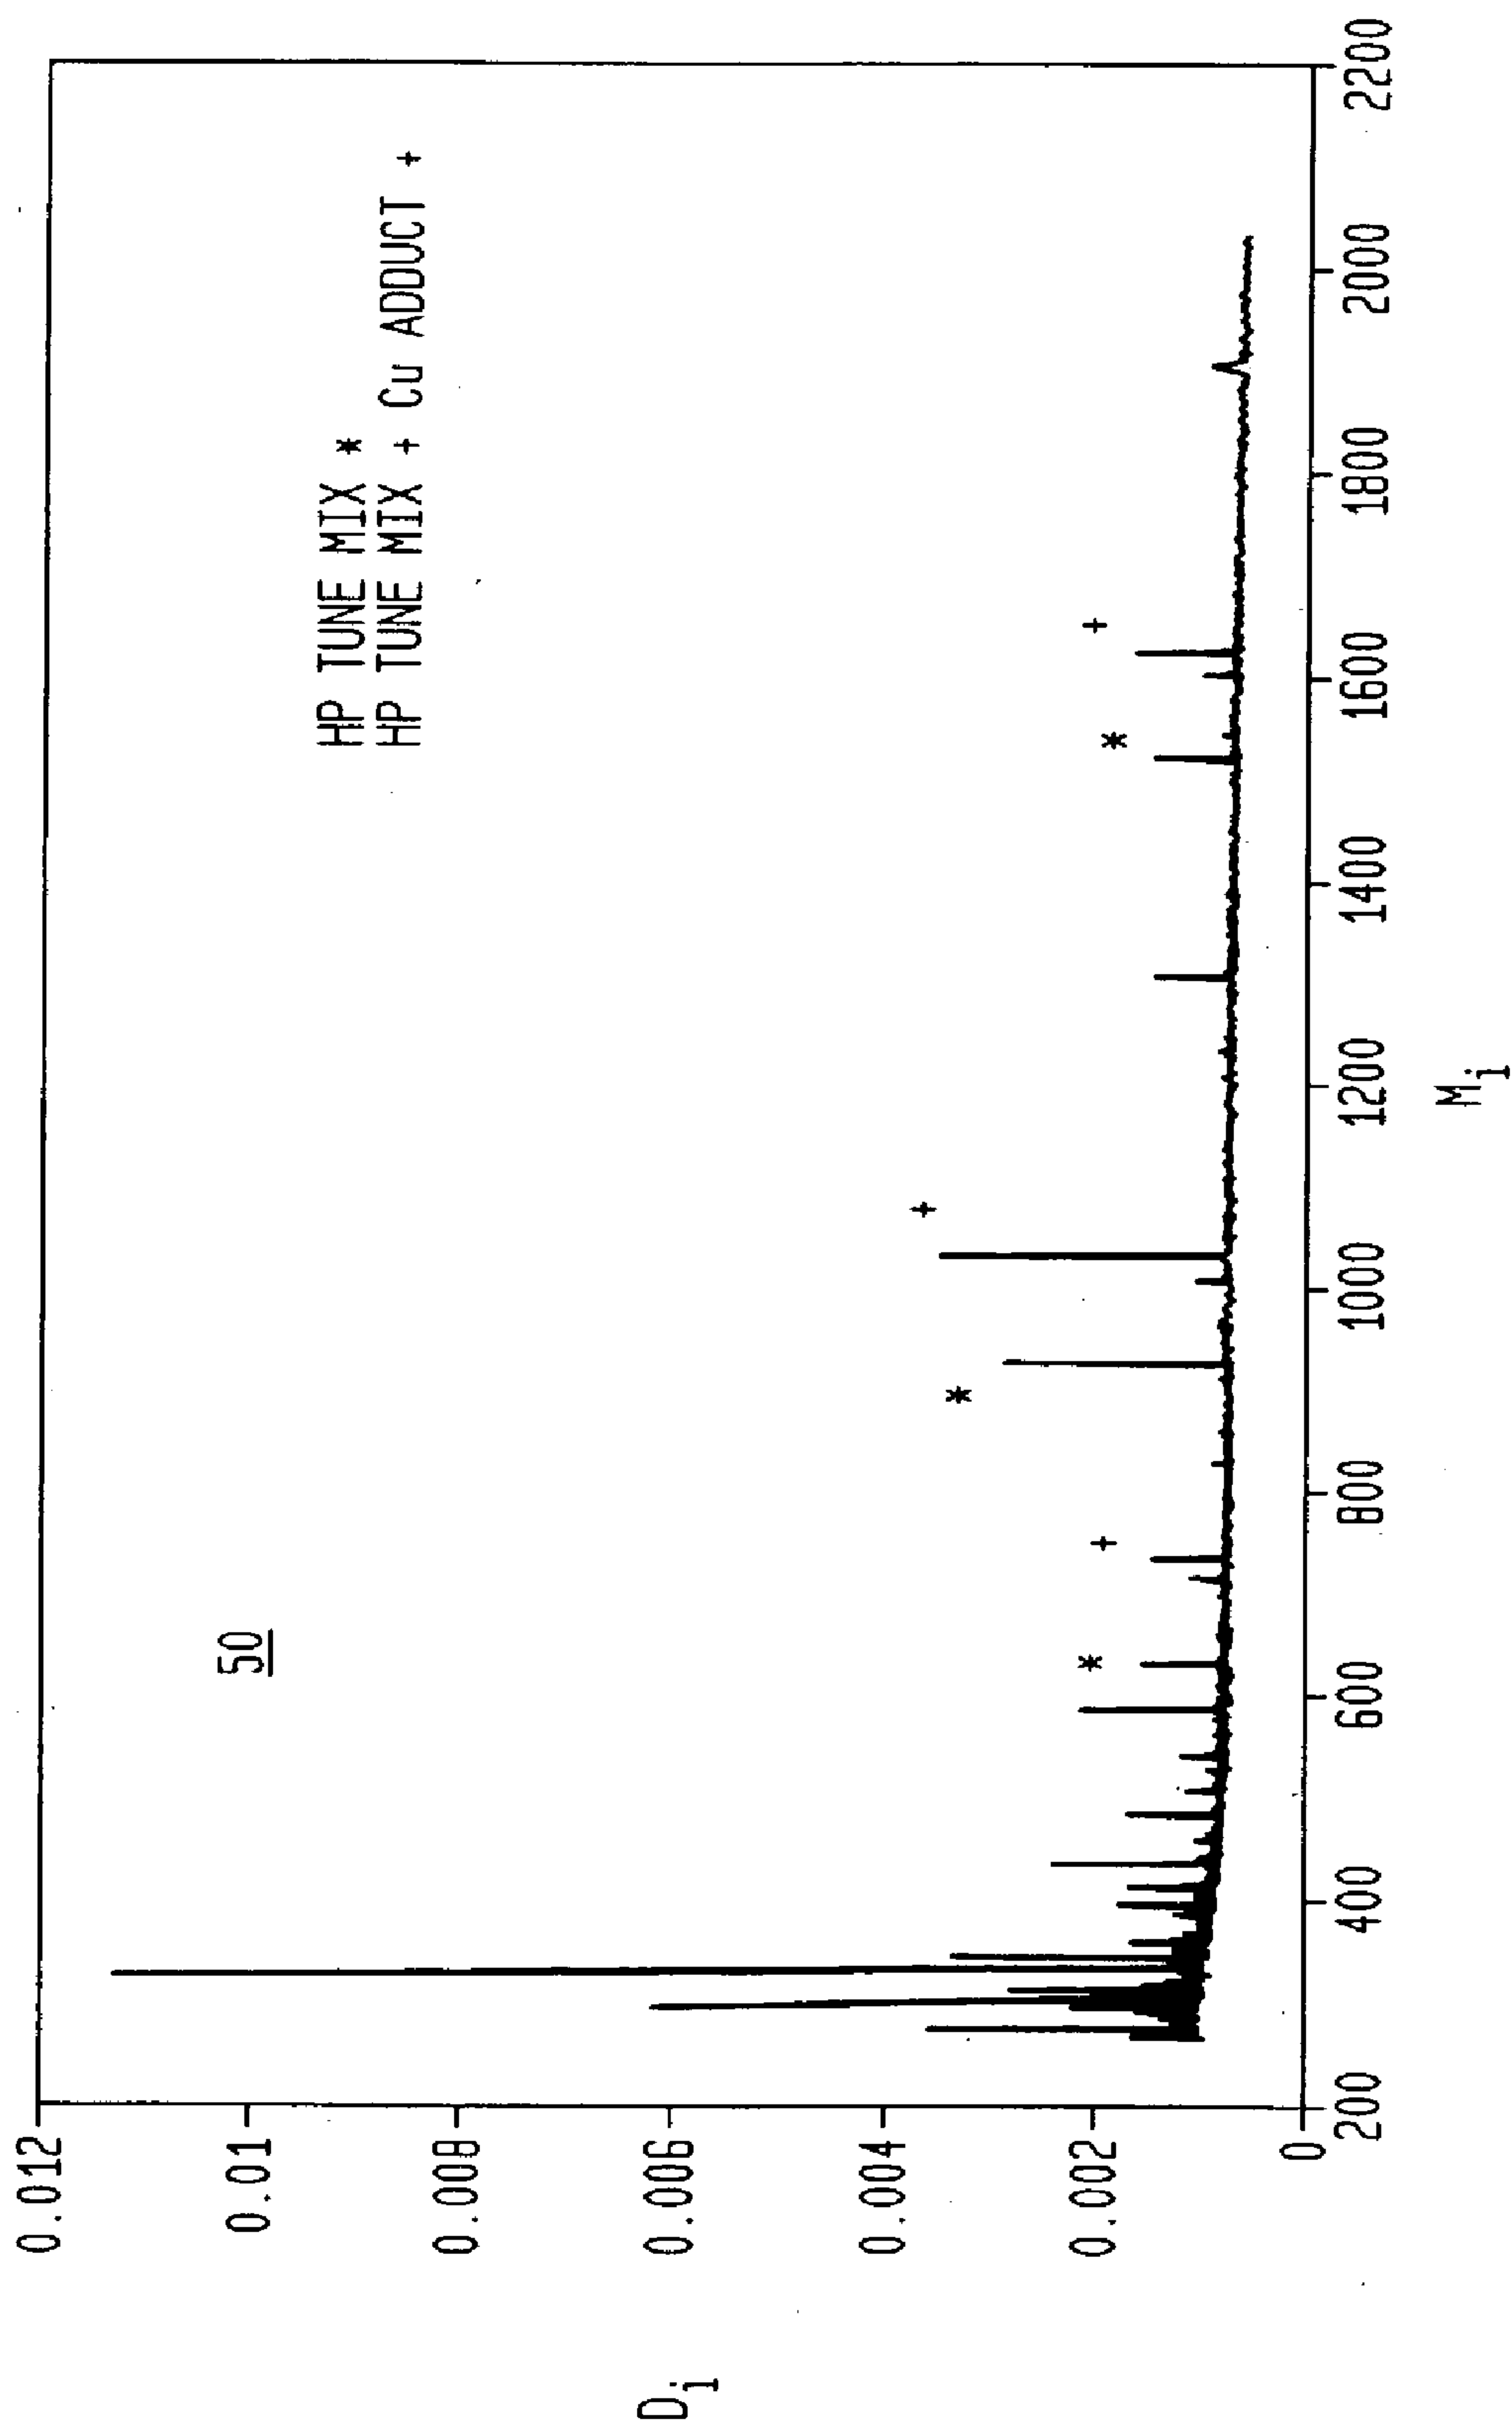


FIG. 11A

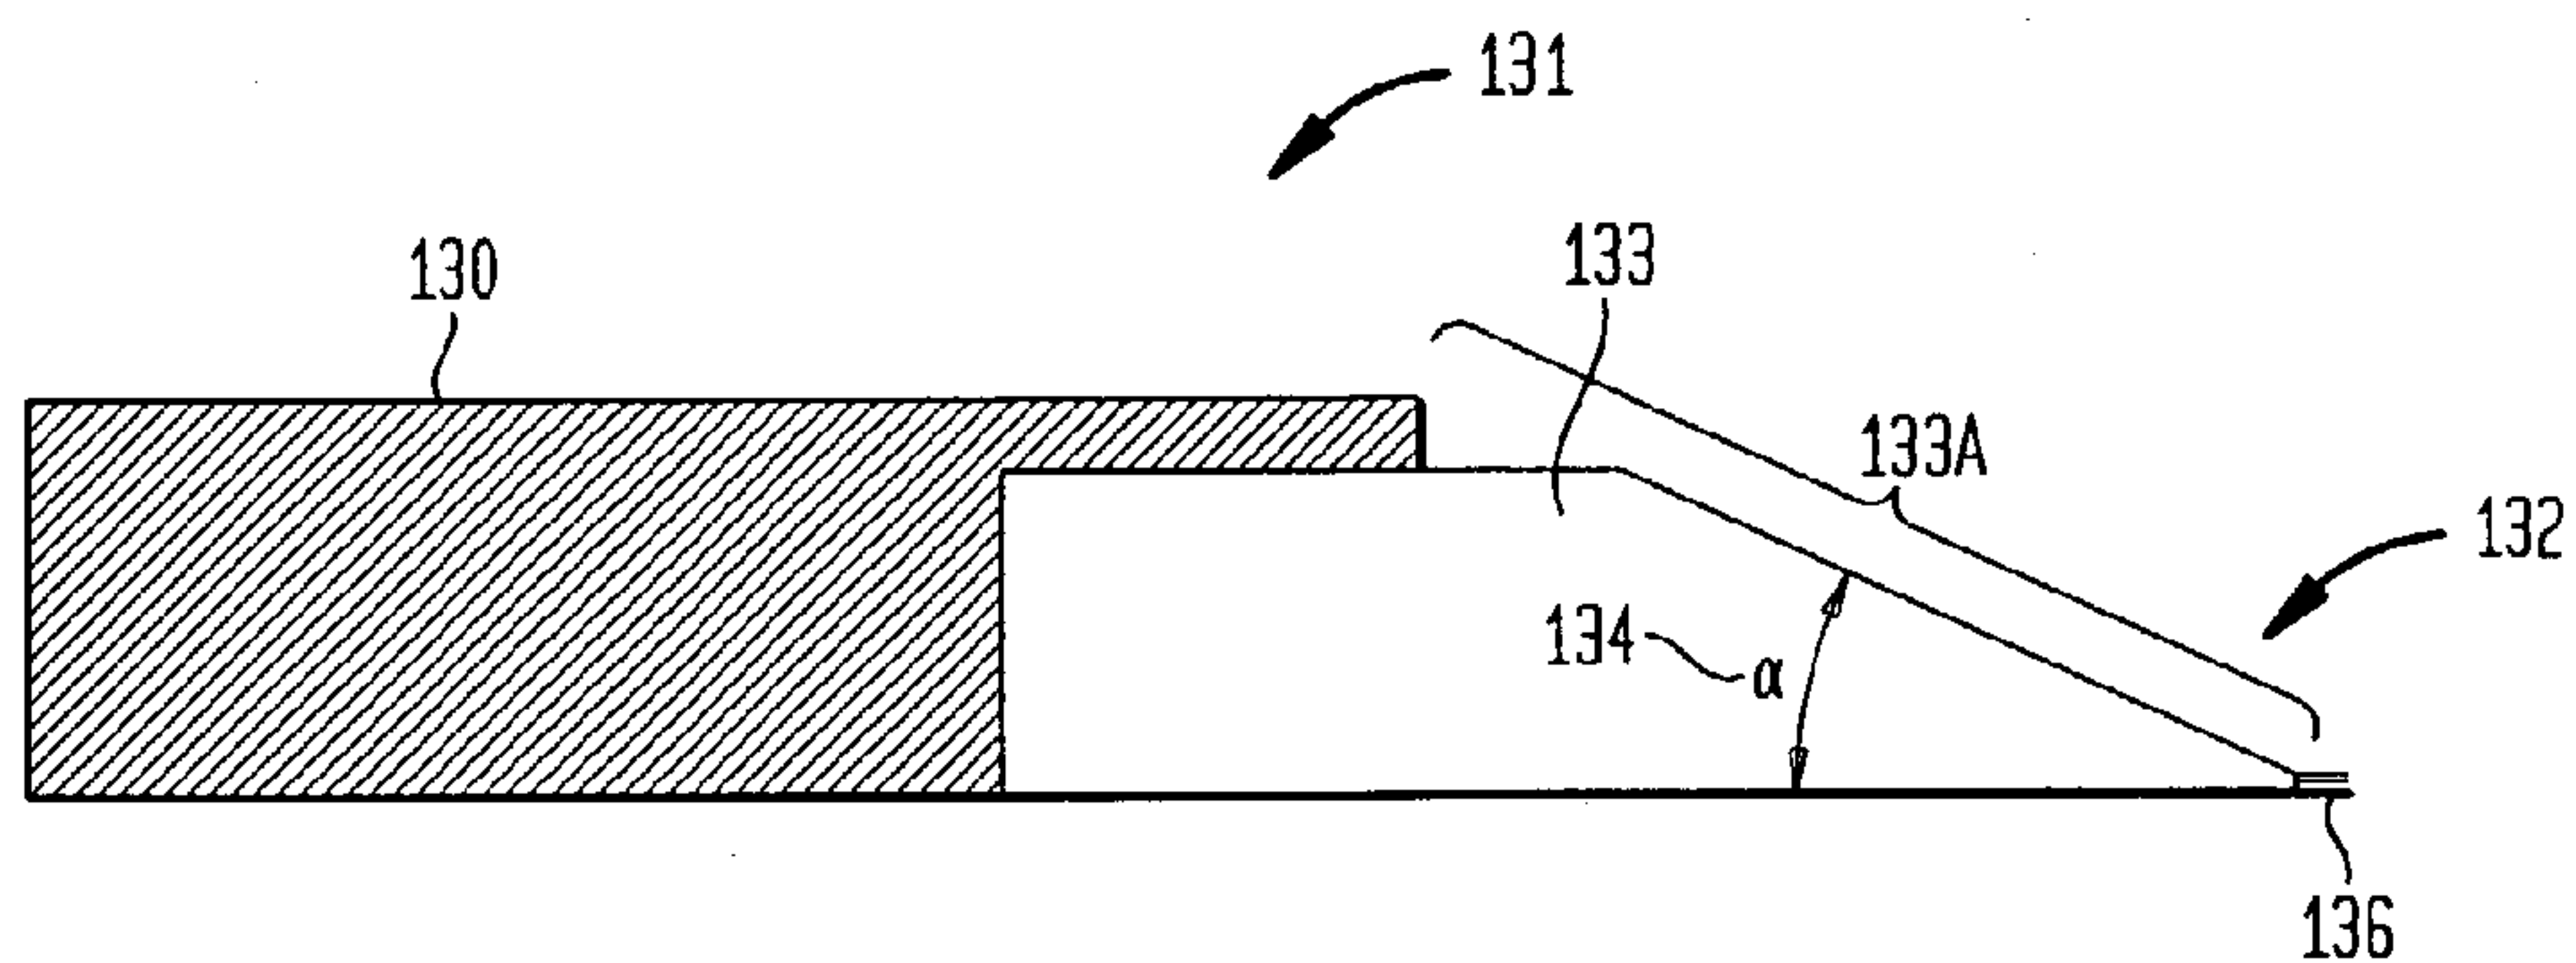


FIG. 11B


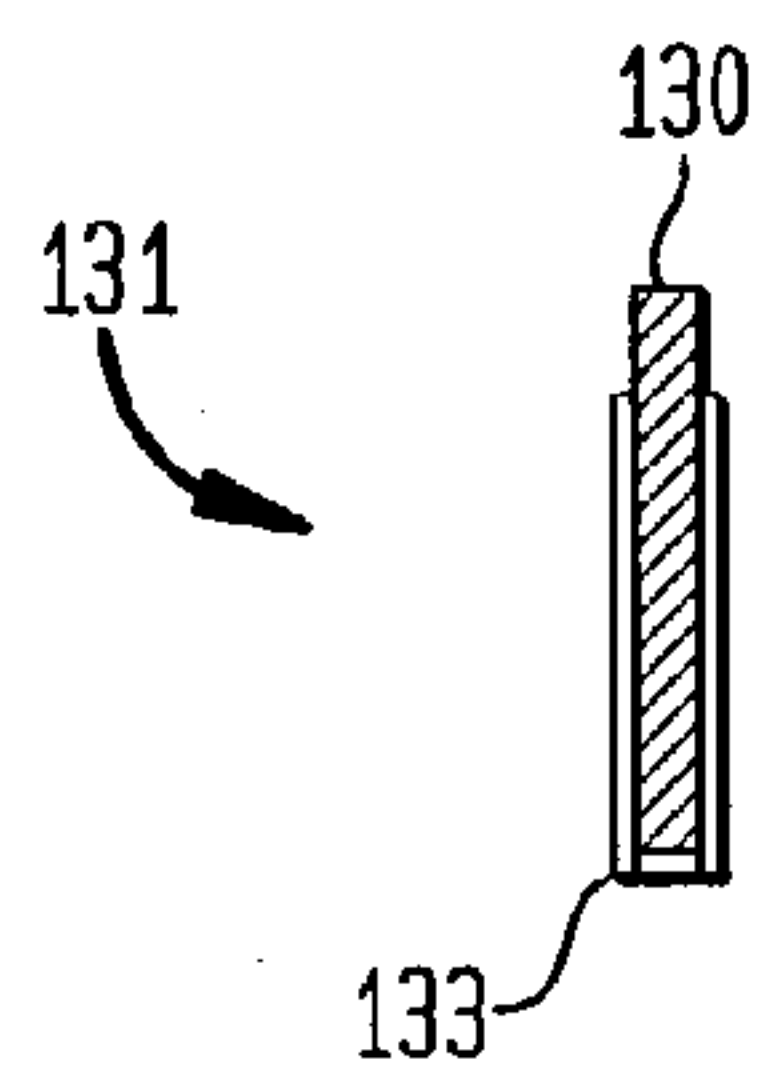


FIG. 11C

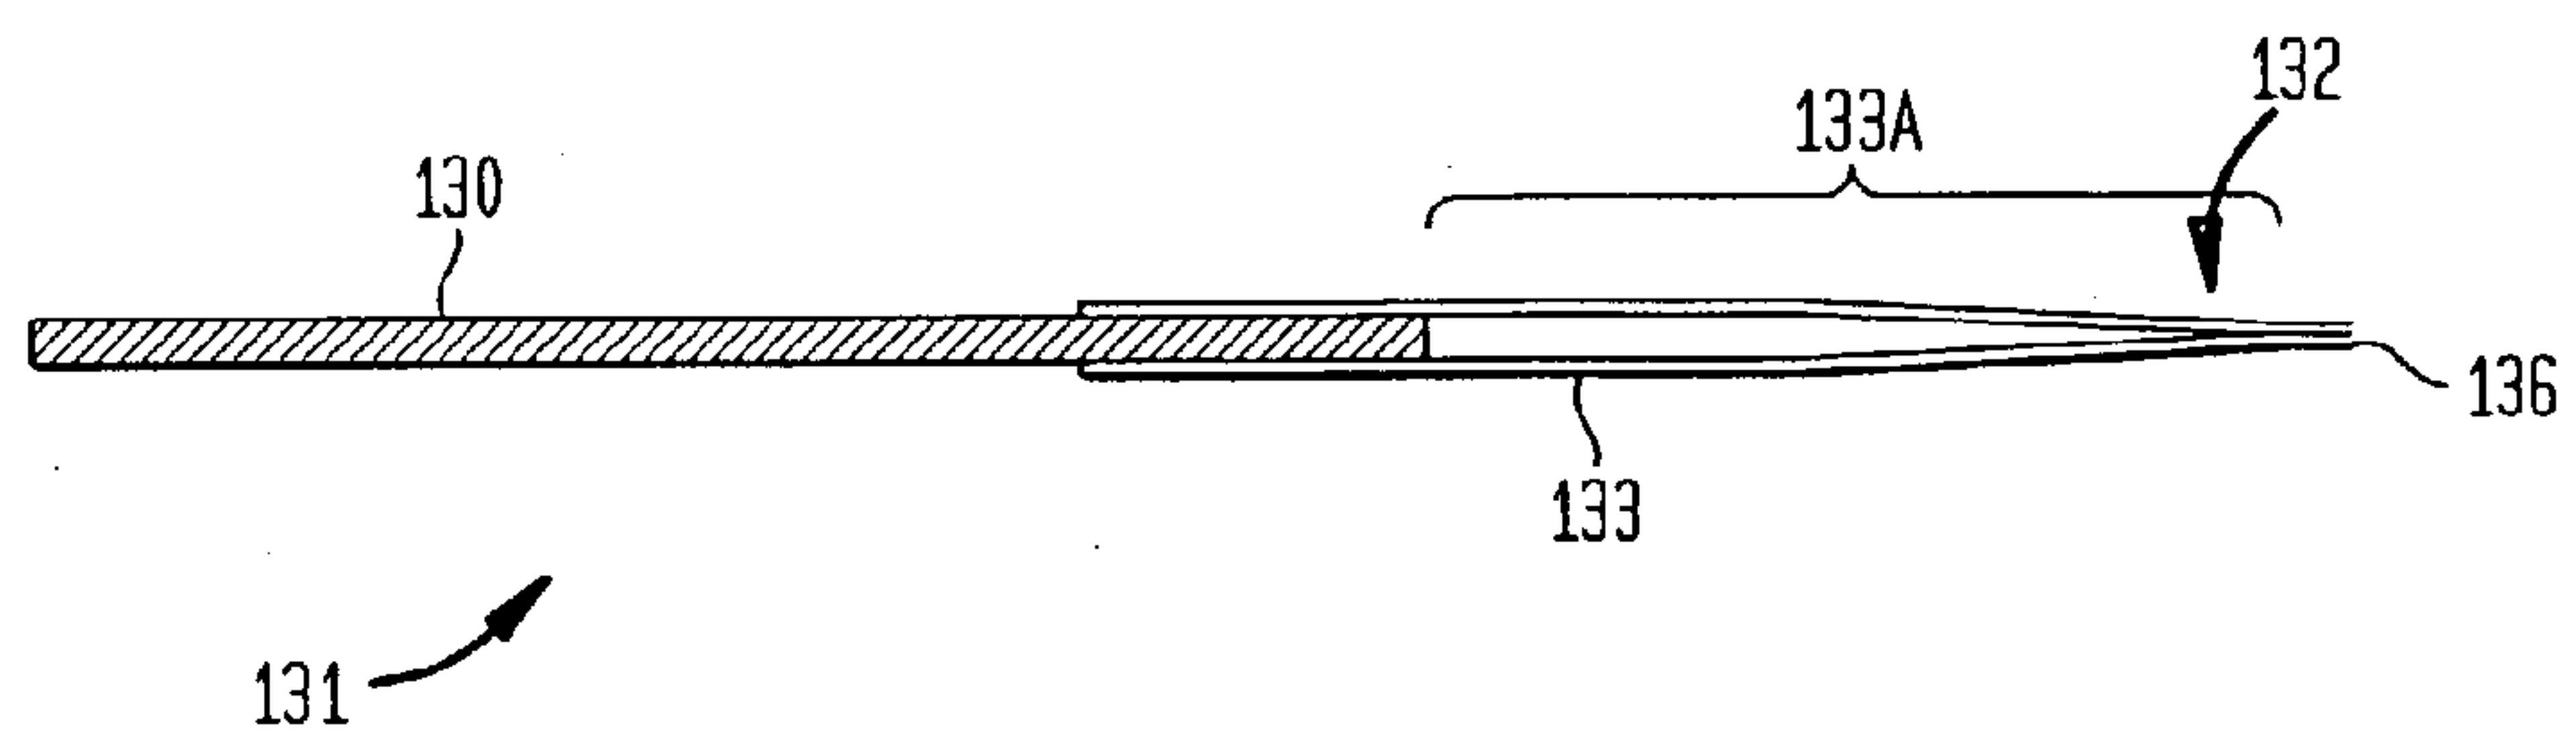

**METHOD AND APPARATUS FOR AN
ELECTROSPRAY NEEDLE FOR USE IN MASS
SPECTROMETRY**

TECHNICAL FIELD OF THE INVENTION

[0001] The present invention relates generally to electro-spray ionization for mass spectrometry, and more particularly the invention relates to an apparatus and method for producing an electrospray from a sample solution for introduction into mass spectrometer.

BACKGROUND OF THE PRESENT
INVENTION

[0002] Mass spectrometry is an important tool in the analysis of a wide range of chemical compounds. Specifically, mass spectrometers can be used to determine the molecular weight of sample compounds. The analysis of samples by mass spectrometry consists of three main steps—formation of gas phase ions from sample material, mass analysis of the ions to separate the ions from one another according to ion mass, and detection of the ions. A variety of means exist in the field of mass spectrometry to perform each of these three functions. The particular combination of means used in a given spectrometer determine the characteristics of that spectrometer.

[0003] The present invention relates to the first of these steps—the formation of gas phase ions from a sample material. More particularly, the present invention relates to electrospray ionization (ESI), one such means for producing gas phase ions from a sample material. Electrospray ionization, was first suggested by Dole et al. (M. Dole, L. L. Mack, R. L. Hines, R. C. Mobley, L. D. Ferguson, M. B. Alice, *J. Chem. Phys.* 49, 2240, 1968). Generally, in the electrospray technique, analyte is dissolved in a liquid solution and sprayed from a needle. The spray is induced by the application of a potential difference between the tip of the needle and a counter electrode. Specifically, a voltage of several kilovolts is applied between, for example, a metal capillary and a flush surface separated by a distance of approximately 20 to 50 millimeters. Under the effect of the electric field, a liquid in the capillary is dielectrically polarized at the end of the capillary. The liquid is then pulled out into a cone, known as the Taylor cone. The surface tension of the liquid at the pointed end of the cone is no longer able to withstand the attraction of the electric field, and this causes a small electrically charged droplet to be detached. The charged droplet flies with great acceleration to the flush counter electrode, effected by the inhomogeneous electric field. During the flight of the liquid, evaporation occurs and the droplets are slowed down. The spray results in the formation of finely charged droplets of solution containing analyte molecules. The larger ions become ionized, and move towards the counter electrode to be transferred into the vacuum system of a mass spectrometer, for example, through a narrow aperture or capillary. Very large ions can be formed in this way. For example, ions as large as 1 MDa have been detected by ESI in conjunction with mass spectrometry (ESMS).

[0004] Electrospray, as in the present invention, facilitates the formation of ions from sample material. It should be noted that the size of the droplets produced in the ESI technique is dependant upon the size of the sprayer used.

The terms nanospray or micro spray are used to indicate the use of very small sprayers in electrospray technique. In other words, a sprayer having an opening of less than about 10 μm (microns) will produce a nanospray, a sprayer having an opening of between approximately 10-100 μm (microns) will produce a micro spray, and a sprayer having an opening of greater than 100 μm (microns) will produce an electrospray. For convenience, all three are referred to generally as “electrospray,” in as much as the present invention can be used with each.

[0005] Referring to FIG. 1, depicted is an ionization source of copending application Ser. No. 09/570,797 which shows an API source for generating ions from a sample for subsequent analysis. As shown, the ionization source 101 comprises spray chamber 1, transfer region 2, first pumping region 5, second pumping region 4, hinge 9, flange 10, and source block 16. During normal operation of the ionization source 101 incorporating an ESI source it is anticipated that numerous other elements may be used within ionization source 101 as shown in FIG. 1. These may include vacuum pump 15, ion transfer devices such as capillary 6 having an entrance end 7, and exit end 19 and inner channel 8, multipole devices such as pre-hexapole 11 and hexapole 12, as well as other ion optic devices such as skimmers 13 and 14 and exit electrodes 17.

[0006] Initially, sample solution is formed into droplets at atmospheric pressure by spraying the sample solution from a spray needle 20 into spray chamber 1. The spray may be induced by the application of a high potential between the tip of spray needle 20 and the capillary entrance end 7 within spray chamber 1. Then, these sample droplets evaporate while in the spray chamber 1 thereby leaving behind sample ions. These sample ions are accelerated or directed toward capillary entrance 7 and into channel 8 by the electric field generated between spray needle 20 and capillary entrance 7. These ions are then transported through capillary 6 to capillary exit 19, due to the flow of gas created by the pressure differential between spray chamber 1 and first transfer region 2.

[0007] The present invention relates particularly to the sprayers used within electrospray ionization. Presently, known electro-spraying techniques teach that it is necessary to take active steps to ionize the solution for analysis in the mass spectrometer. For instance, FIG. 2 depicts a typical prior art electrospray needle 21. As shown, needle 21 comprises an elongated capillary structure tapered at one end to form tip 22. Needle 21 includes a plenum 24 to receive the liquid sample. Plenum 24 is shown having an interval region larger than that of the capillary section of needle 21. Liquid sample flows from plenum 24 through upstream inlet 25 into the capillary section of ejection through tip 26. Plenum 24 may be electrically conductive so that a voltage applied to the plenum 24 will allow for the transfer of charge into the liquid stream. Alternatively, a charge can be imposed on the capillary section of needle 21. The applied voltage produces an electrical field which is arranged such that it is at its highest at the tip 26 such that the charge and field at tip 26 are high enough to form the electrospray (i.e. charged droplets). Such a prior art apparatus consists only of a single needle which, is a very thin capillary, producing flow rates on the order of 20 nL/min. Further, such a needle must be loaded through its back end

(i.e. the plenum **24**, as shown in **FIG. 2**), not through the tip **25**. This can be a very time consuming process.

[0008] Typically, nanospray needles are produced by taking a glass capillary having a relatively large diameter and pulling and/or machining it to a tip. Then a metal coating is vapor deposited onto its outer surface, as disclosed in Mann U.S. Pat. No. 5,504,329 (Mann). The needle shown in **FIG. 3** is the result of such a process. Needles such as this are formed by using heat to soften glass capillary tubing and pulling the tip end to form the needle's tapered tip **27**. These needles are generally single use, and must be loaded with sample solution using micropipettes or some other means for loading sample solution through the end **28** of the needle—the end opposite the spray tip—using a micropipette.

[0009] Such needles are generally single use, and require the sample to be reloaded through its back end after each use. The prior art needles breed inaccuracy because the conditions have to be replicated with each removal and replacement. In addition, the fragile nature of the needles, combined with their limited use, makes replacement costs a significant expense for their users. Also, because these needles are extremely fragile, replacement is frequent, which is both costly and time consuming.

[0010] Once these prior art needles are formed, a means of making electrical contact is required. Prior art needles have been made from small metal tubing (e.g., a steel syringe needle) or dielectric tubing (e.g., glass, fused silica or polymer tubing). If the needle is made of an insulating material, there are generally three ways that the prior art teaches to make a needle capable of electrical contact: (i) applying thin metal films directly onto the dielectric tubing, (ii) supporting the dielectric tip inside a secondary metal tube that contacts the liquid as it exits the dielectric tubing and (iii) making a direct electric contact with the solution from a remote position. The most commonly used of these is the application of a thin metal film (e.g., gold or platinum) directly onto the dielectric tubing.

[0011] However, due to their relatively inert nature, such metals often show poor adhesion to the substrate materials, which reduces ESI stability and eventually leads to ESI tip failure. As the analyte is sprayed from the tip, the metal coating can rapidly deteriorate through peeling or flaking. An attempted solution to this problem has been to apply an interlayer material, such as chromium or sulfur containing silanes, which adheres to both the metal and the substrate. However, this has not entirely solved the problem because such interlayer materials are subject to chemical attack (i.e., dissolution, in the case of chromium, or bond cleavage, in the case of silanes).

[0012] Valaskovic U.S. Pat. No. 5,788,166 (Valaskovic), for example, uses a process of applying a metal overcoating on a dielectric capillary needle. The capillary needle is constructed by heating fused-silica tubing with a laser, then pulling the tube until its internal diameter is in the range of 3 μm . The pulling process is followed by chemical etching and surface metallization. The pulling results in formation of slowly tapered capillary edges and a tip having a very small inner diameter. The chemical etching process forms the tapered outer wall and a sharp point at the tip of the needle. The surface metallization applies a thin metal contact layer on the outer wall of the needle, to allow for electrical contact. Then an electrically insulating overcoat is applied.

The overcoat essentially fixes the conductive metal contact layer into place, although the electrically insulating overcoat does not improve the adhesion of the metal to the capillary.

[0013] Because the pulling process is used on fused silica tubing, the extra step of metallization is required. The pulling process results in slowly tapered edges, which culminate in a sharp point. This point is then etched to create a narrow diameter opening at the distal end (or tip) of the pulled tubing (i.e., forming a needle). A needle such as this has the disadvantage of the formation of “bubbles” in the solution within the needle, which interferes with the spray of the solution—in fact, it may even stop flow of the solution from the needle. In other words, having such a narrow diameter at the distal end (or tip) of the needle permits air pockets to form at the base of the tip. That is, solution near the distal end may begin to evaporate, thereby forming air pockets. These air pockets then permeate through the solution toward the proximal end (due to the larger space available), effectively “blocking” the spray of solution from the needle. The glass structure of the needle also contributes to the formation of these air pockets, as the solution is held within the needle due to capillary action. In other words, the solution grips the inner surface of the needle as the air pockets permeate through the interior of the needle.

[0014] Other forms of electrospray include pneumatic assisted, thermal assisted, or ultrasonic assisted, or the addition of arc suppression gases so that higher voltages can be applied during electrospray formation. Pneumatically assisted sprayers typically have a much larger tip (greater than 100 μm) than, for example, nanosprayers (around 5 μm) (See **FIG. 4** for an example of a nanospray needle). When using pneumatically assisted sprayers, sample solution is typically pumped (for example, via a syringe pump) into the sprayer. Sample aliquots can then be injected into this solution stream either manually or automatically (i.e., by a robot or other machine). However, the conventional process of injecting sample into sprayers by machines is cumbersome, as the process is difficult to control. That is, filling the needle through its proximal end is not practical—since the opening at the proximal end is so small. The glass capillary, with the opening at the end, provides a measure of resistance during filling, and therefore must be performed carefully with a micropipette.

[0015] Accordingly, prior to the present invention, a need has existed for a multiple use, robust, spray needle and sprayer having a geometry that eases the elimination of voids or bubbles. It is a purpose of the invention to provide such a spray needle and sprayer, as well as a method of operating a mass spectrometer using a spray needle and sprayer to produce an electrospray formed from a sample solution. It is also a purpose of the present invention to provide a means and method of operating a mass spectrometer which utilizes the apparatus with a variety of ionization techniques (i.e., ESI, MALDI, etc.)

SUMMARY OF THE INVENTION

[0016] One aspect of the present invention is to provide an apparatus and method of facilitating the introduction of a liquid sample into a mass spectrometer for subsequent analysis. To address the foregoing problems, the present invention provides a sprayer which is reusable, robust, and easy to load. Furthermore, the present invention provides a

spray needle and sprayer which has a geometry that minimizes the formation of voids or bubbles, thereby providing improved results in the analysis of the sample solution, as demonstrated in the mass spectra of **FIG. 10** obtained in a mass analysis performed using the spray needle according to the preferred embodiment disclosed herein.

[0017] Specifically, one embodiment of the present invention comprises a two component spray needle (i.e., a support and a tip). Advantages of a spray needle having this configuration include ease of sample loading, minimization of bubble formation or voids, durability, reusability, ease of automation, ease of replacement, increased reproduction of analysis results, etc. For example, if after repeated uses the tip is no longer functional, a new tip may be constructed, and attached to the intact support.

[0018] Another embodiment of the present invention provides a single component spray needle and sprayer having an opening along its length to facilitate the introduction or loading of a sample solution into the needle. In other words, the spray needle can be filled with the solution through its an elongated slit along its length by merely dipping the needle into the sample solution. This allows for the liquid to be drawn in through the tip into the body of the spray needle via capillary action. At the same time, this may limit the droplet size upon ejection of the sample from the needle. The opening also provides for unique spraying capabilities due to its geometry and length. Furthermore, because the spray needle does not need to be loaded via the rear opening (or proximal end), the spray needle can be easily employed within automated systems.

[0019] Yet another embodiment of the present invention comprises a single unit spray needle having a slit along its length as well as having the tip end diagonally cut (as shown in **FIGS. 7A-7C**). The construction of this embodiment provides a robust needle which facilitates the introduction of sample solution into the spray needle through its proximal end (or tip) as well as facilitates the production of very small sample droplets for ionization. In addition, the spray needle of this embodiment can be loaded through a dipping process, making it ideal for use with an automated process. The needle of this embodiment also minimizes the formation of bubbles or voids in the sample solution.

[0020] Yet a further embodiment of the invention comprises a multi-tip spray needle (as shown in **FIGS. 11A-C**). Such a spray needle preferably embodies the structure of the preferred embodiment shown in **FIGS. 5A-C**, but alternatively, may embody the alternative structures shown in **FIGS. 6A-C** and **7A-C**. Specifically, a multi-tip spray needle according to the invention may comprise a plurality of (e.g., 20, 50, 100, etc.) very fine (i.e., on the order of 50 μm or less) elements at the needle's distal end. An advantage of such a multi-tip structure is the facilitation of the spray of extremely fine droplets, having the effect of maximizing the introduction of sample ions into the mass analyzer from the source region.

[0021] Other objects, features, and characteristics of the present invention, as well as the methods of operation and functions of the related elements of the structure, and the combination of parts and economies of manufacture, will become more apparent upon consideration of the following detailed description with reference to the accompanying drawings, all of which form a part of this specification.

BRIEF DESCRIPTION OF THE DRAWINGS

[0022] A further understanding of the present invention can be obtained by reference to a preferred embodiment set forth in the illustrations of the accompanying drawings. Although the illustrated embodiment is merely exemplary of systems for carrying out the present invention, both the organization and method of operation of the invention, in general, together with further objectives and advantages thereof, may be more easily understood by reference to the drawings and the following description. The drawings are not intended to limit the scope of this invention, which is set forth with particularity in the claims as appended or as subsequently amended, but merely to clarify and exemplify the invention.

[0023] For a more complete understanding of the present invention, reference is now made to the following drawings in which:

[0024] **FIG. 1** depicts an atmospheric pressure ionization (API) source block for introducing ions from an ionization source (e.g., ESI, etc.) into a mass analyzer for subsequent analysis;

[0025] **FIG. 2** shows a lengthwise cross-sectional view of a prior art nanospray needle as shown in Myers U.S. Pat. No. 5,975,426;

[0026] **FIG. 3** shows a lengthwise cross-sectional view of a prior art nanospray needle according to Mann U.S. Pat. No. 5,504,329;

[0027] **FIG. 4** is a microphotograph showing a prior art nanospray needle;

[0028] **FIG. 5A** shows a side view of a preferred embodiment of a spray needle according to the present invention;

[0029] **FIG. 5B** shows an end view of the spray needle depicted in **FIG. 5A**;

[0030] **FIG. 5C** shows a top plan view of the spray needle depicted in **FIG. 5A**;

[0031] **FIG. 6A** shows a top plan view of an alternate embodiment of the spray needle in accordance with the present invention;

[0032] **FIG. 6B** shows an end view of the spray needle shown in **FIG. 6A**;

[0033] **FIG. 6C** shows a side view of the spray needle shown in **FIG. 6A**;

[0034] **FIG. 7A** shows a top plan view of another alternate embodiment of the spray needle according to the present invention;

[0035] **FIG. 7B** shows a side view of the spray needle shown in **FIG. 7A**;

[0036] **FIG. 7C** shows an end view of the spray needle shown in **FIG. 7A**;

[0037] **FIG. 8** depicts the electrospray needle shown in **FIGS. 5A-C** integrated within an electrospray assembly according to the present invention;

[0038] **FIG. 9** depicts the electrospray assembly showing in **FIG. 8** integrated into an ionization source block;

[0039] FIG. 10 shows a mass spectra obtained in a mass analysis performed using the spray needle of FIGS. 5A-C in accordance with the present invention; and

[0040] FIG. 11A shows a side view of a yet another alternate embodiment of a spray needle according to the present invention;

[0041] FIG. 11B shows an end view of the spray needle depicted in FIG. 11A;

[0042] FIG. 11C shows a top plan view of the spray needle depicted in FIG. 11A.

DETAILED DESCRIPTION OF A PREFERRED EMBODIMENT

[0043] As required, a detailed illustrative embodiment of the present invention is disclosed herein. However, techniques, systems and operating structures in accordance with the present invention may be embodied in a wide variety of forms and modes, some of which may be quite different from those in the disclosed embodiment. Consequently, the specific structural and functional details disclosed herein are merely representative, yet in that regard, they are deemed to afford the best embodiment for purposes of disclosure and to provide a basis for the claims herein which define the scope of the present invention. The following presents a detailed description of a preferred embodiment (as well as some alternative embodiments) of the present invention.

[0044] Referring initially to FIG. 5A, shown is a side view of a preferred embodiment of spray needle 31 according to the present invention. As shown, spray needle 31 according to the preferred embodiment of the invention comprises two component parts, support 30 and foil 33.

[0045] Support 30 is preferably constructed from a rigid and electrically conductive material (e.g., steel, etc.). It is also preferred that the support 30 be a solid yet thin structure (i.e., on the order of 400 μm or less in thickness). The thickness of the support contributes to the determination of the loading and spray properties of the sprayer (i.e., how fast the solution will flow into the sprayer, the potential at which the sprayer must be operated, the optimal distance between the sprayer and ESI orifice, and the solution flow rate during spray etc.), because the thickness of support 30 determines the size of foil 33. It is further preferred, as shown in FIG. 5B, that support 30 have a rectangular cross section. This geometry eases the elimination of voids or bubbles which interfere with the spray of the solution. Alternatively, support 30 may have a different cross-sectional shape (e.g., triangular, circular, hexagonal, etc.). Such change in the shape of support 30, however, may alter the spray properties of the sprayer. Thus, different structures may be ideal for different sample solutions.

[0046] Generally, foil 33 may be constructed using a piece of electrically conducting "foil" which is cut at an angle α , as shown in FIG. 5A. In the preferred embodiment, the foil 33 is attached to the outer surface of support 30 and is in direct contact with a portion of one end of support 30, as depicted in FIGS. 5A and 5C. Foil 33 is attached such that it is in electrical contact with support 30. Preferably, an adhesive is used to attach foil 33 to support 30, but other means for attaching the foil 33 to support 30 may be used, such as soldering. Foil 33 is preferably constructed from a chemically inert and easily cleaned material (e.g., gold,

copper, platinum, stainless steel (because of its limited reactivity to certain compounds), etc.). For example, certain species are not readily protonated, but will accept, for example, silver or copper ions as adducts. Therefore, use of such different materials for foil 33 may alter the life and spray properties of the spray needle 31 (i.e., durability, sample loading flow rate, the potential at which the spray needle must be operated, the optimal distance spray needle 31 is positioned from the capillary orifice (see FIG. 9), the spray flow rate, etc.)

[0047] Alternatively, other materials might be used in the construction of foil 33, depending on the particular electrochemical or reactive properties desired. For example, the utilization of copper instead of gold as the material for foil 33 will result in the formation of copper ions, and has the potential for forming complexes with analyte species. Some of such complexes have been known to enhance signal intensity in certain analyses.

[0048] Preferably, foil 33 is constructed from a very thin piece of metal (i.e., about 100 μm in thickness). However, the thickness of foil 33 may be chosen such that needle 31 obtains certain properties (i.e., durability, formation, spray type, etc.). In fact, the choice of thickness of foil 33 may depend on the material from which foil 33 is constructed (e.g., gold, copper, etc.).

[0049] In the preferred embodiment of the spray needle 31 of the present invention as shown in FIGS. 5A-5C, tip 32 may be formed by wrapping or folding a portion of foil 33 around a portion of support 30 and adhering foil 33 to support 30. Once wrapped or folded, the exposed end of foil 33 is preferably cut at an angle α 34, as shown in FIG. 5A, thereby forming tip 32. Foil 33 is preferably attached to support 30 in such a way that it conforms to the shape of support 30 (e.g., if support 30 is rectangular, then foil 33 would conform to this rectangular shape (i.e., it would resemble a straight edged 'U' shape)).

[0050] Alternatively, support 30 may comprise an opening on one of its ends for accepting an end of foil 33 and securing foil 33 therein. Among other things angle α 34 and the thickness of foil 33 each contribute to the determination of the loading and spray properties of the sprayer (i.e., the rate at which the solution will flow into the sprayer, the potential at which the sprayer must be operated, the optimal distance between the sprayer and ESI orifice, and the solution flow rate is during spray, etc.) Preferably, angle α 34 is approximately 45 degrees. This provides optimum performance of the spray needle 31 during operation. Of course, angle α 34 may be any angle between zero and ninety degrees, but importantly, the specific angle α 34 used will affect the properties and/or performance of spray needle 31. Specifically, angle α 34 aids in determining the flow rate of the spray, and, in turn, the accuracy and exactness of the mass analysis results. Also, choice of angle α 34 for optimum results may vary in accordance with the sample or technique being used, the material used for foil 33, the potentials being applied, the distance between the needle 31 and the ESI orifice, etc.

[0051] Of course, the relative dimensions of support 30 and foil 33 may differ from that shown in FIGS. 5A-C. Specifically, the geometry of support 30 (and therefore the assumed geometry of foil 33 when attached to support 30) may differ from the geometry of foil 33 at the spraying end.

For example, foil **33** at support **30** as shown in **FIG. 5A**, is rectangular, while foil **33** at tip **32** may be slightly “crushed” so as to produce a gap narrower than the thickness of support **30**. Although this may reduce the solution flow rate throughout the sample loading and spray process, it will importantly allow for the spray of smaller droplets of the sample solution during the ESI process and result in enhanced performance of the ESI.

[0052] The construction of the apparatus and attachment of foil **33** to support **30** is unique because the opening in the resulting invention is along the length. This allows sample to be loaded into the needle **31** anywhere along the aperture (as indicated by **33A**) along its length by a simple dipping process. Further, the needle **31** maintains the ability to produce very small droplets (or larger ones), can be extremely robust, is reusable, convenient for use in fully automated systems, etc.

[0053] More specifically in the preferred embodiment shown in **FIGS. 5A-C**, the sample solution may be loaded into needle **31** aperture **33A**. To load the sample, the invention may be held vertically, and tip **32** lowered into a sample solution. The sample solution will be drawn into foil **33** via capillary action, thereby filling the internal cavity within foil **33** (created when foil **33** is wrapped or folded around support **30**). Due to the ease of filling foil **33** with sample, and its heightened durability over prior art needles, the invention may be repeatedly cleaned and reused.

[0054] This reusability, coupled with the geometric structure of the needle (which eases the elimination of interfering voids or bubbles) may be especially important in an alternative embodiment which utilizes the invention for the fully automated analysis of samples in conjunction with a robot. Another variation uses the invention to accomplish sequential analysis of a multitude of samples.

[0055] Importantly, use of a spray needle according to the preferred embodiment disclosed herein provides improved results in the analysis of a sample solution, as demonstrated by the mass spectra **50** shown in **FIG. 10** obtained in a mass analysis performed using the spray needle according to the preferred embodiment.

[0056] Referring next to **FIGS. 6A-6C**, shown is an alternate embodiment of a spray needle **41** in accordance with the present invention. In particular, shown in **FIG. 6A** is a top plan view of spray needle **41** comprising an elongated structure having an inner channel there through. Spray needle **41** further includes a tapered end **36** which culminates into an opening at tip **42**. This embodiment of the invention further comprises an opening **35** (or slit) which extends along substantially the entire length of needle **41** (i.e., from tapered end **36** all the way to the other end of needle **41**). Of course, optionally, the opening **35** may extend for only a short part of needle **41**. Also, opening **35** may be a series of holes or openings aligned lengthwise along needle **41** rather than a single continuous slit, as shown. Opening **35** (or a series of openings) provides the user with an improved method of loading the sample solution into the spray needle, as well as providing a variety of options as to controlling the spray of the sample from the needle. For example, opening **35** provides a greater area for the sample to be drawn into the spray needle **41**, and therefore enhances the loading characteristics and abilities of needle **41**. That is, needle **41** may be loaded quickly and efficiently, allowing the user to load sample via an automated process.

[0057] As shown, needle **41** is preferably cylindrical in structure. Of course, other structures may be used (i.e., rectangular, square, triangular, etc.). It is also preferred that needle **41** be constructed from a solid, yet thin material (i.e., on the order of 400 μm or less in thickness). It is also preferred that needle **41** include an opening at tip **42** having a diameter (if needle **41** is cylindrical) of between about 20 μm and 50 μm . Alternatively, needle **41** may be used in a nanospray ionization source, and therefore would preferably include an opening at tip **42** having a diameter (if needle **41** is cylindrical) of approximately 5 μm . As the above demonstrates, the opening in tip **42** determines the spray properties of the needle (i.e., flow rate etc.).

[0058] Turning next to **FIG. 7A**, shown is a top plan view of yet another alternate embodiment of a spray needle according to the present invention. Specifically, shown is spray needle **43** comprising an elongated body **42** (shown here as being cylindrical, but other shapes may be used) having an inner channel therethrough. Spray needle **43** further includes an opening **39** along the length of body **42** is cut at an angle **44** (as shown in **FIG. 7C**) such that a substantial opening **37** is created at the spray end of needle **43**. Also, opening **37** is such that a narrow sharp tip **38** is created at the end of needle **42**. Tip **38** provides a means for distributing sample droplets in a variety of different sizes (i.e., a larger opening at tip **38** would produce larger droplets). For example, a high electric field maintained at tip **38** may result in the solution being discharged from tip **38** in the form of a Taylor Cone.

[0059] The embodiments of a spray needle according to the invention shown in **FIGS. 5-7** may also be treated on the internal area of the spray end of the needle of **FIGS. 5A, 6A** or **7A** with polypropylene or some other polymer coating. This treatment allows a needle to be more readily cleaned, while not interfering with the functionality of the needle. Further, this treatment makes the inner surface of the needles spray end inert with respect to the sample solution being tested and will therefore prevent any negative effects which may be caused by the substance used for the body of the needle (i.e., gold, copper, stainless steel, etc.).

[0060] Turning next to **FIG. 8**, shown is one embodiment of the integration of the spray needle of **FIGS. 5A-C** within an electrospray assembly according to the present invention. Of course, similarly, the alternative embodiments of a spray needle according to the invention (i.e., as shown in **FIGS. 6A-C, 7A-C** and **11A-C**) may be integrated with an electrospray assembly as shown in **FIGS. 8** and **9**. As shown, hole **105** in entrance cap **97** is designed especially to receive the tip of spray needle **93**. During operation, spray needle **93** and entrance cap **97** are at different electrical potentials—by about 1000 V. It is this potential difference which induces the spray process. However, the strength of the field at tip **104** of spray needle **93** is of critical importance in producing a spray and subsequently ions. The potential difference between needle **93** and cap **97** might be 1000 V without inducing a spray. If needle **93** is too far from entrance cap **97** then the field strength at tip **104** of needle **93** will be too low and no spray will be formed. If needle **93** is too close to entrance cap **97** then an arc will form between needle **93** and cap **97**—and no spray will be formed. Hole **105** of entrance cap **97** is designed to ease the positioning of needle **93** with respect to cap **97**. Because hole **105** is cylindrical and significantly greater in length than in diameter, tip **104** of

needle **93** can be located in a range of positions in hole **105** without great influence on the strength of the field at tip **104**. That is, because hole **105** is cylindrical, there is a range of positions along the axis of hole **105** within which the distance between these positions and the nearest point on the surface of hole **105** is a constant. Assuming the potential difference between cap **97** and needle **93** is a constant, and the distance between tip **104** and cap **97** is a constant within the above mentioned range of positions, the strength of the field at tip **104** will also be a constant.

[0061] The positioning of needle **93** with respect to capillary section **98** (as seen in **FIG. 9**) is thus one dimensional (i.e., along the longitudinal axis **106** of needle **93**). The position of needle **93** is fixed in the plane perpendicular to axis **106** by the mechanical alignment of components **91** through **100** in assembly **90**. Along axis **106**, there is a range of needle positions over which spray and ions are readily formed. It has been observed that needle **93** should extend approximately 7 mm (+/-1 mm), from the end of retainer **96** in order to provide a useable ion current.

[0062] The positioning of needle **93** is eased further in that needle **93** is positioned within assembly **90** independent of the remainder of the source and instrument. That is, to exchange spray needles and/or samples, assembly **90** is first extracted from the source. Then, on the bench, base **91**—together with union **94**, retainer **96**, and needle **93**—is extracted from assembly **90**. Retainer **96** is loosened by partially unscrewing it thus allowing needle **93** to be removed. A new nanospray needle is produced or obtained from a manufacturer. Analyte solution is loaded into the new needle via micropipette from the distal end of the needle. The new needle **93** is then inserted into retainer **96** so that it extends about 7 mm, +/-1 mm, beyond retainer **96**. Retainer **96** is then tightened, and base **91**—together with union **94**, retainer **96**, and needle **93**—is reinserted into cylinder **92** to complete assembly **90**. Assembly **90** is finally reinserted into the source.

[0063] An embodiment of the complete assembly **90**, as inserted into spray chamber **240**, is depicted in **FIG. 9**. Notice that spray chamber cover **107** includes a number of ports, three of which—**108**, **109**, and **110**—are shown. This spray chamber is designed in accordance with co-pending application IONIZATION CHAMBER FOR ATMOSPHERIC PRESSURE IONIZATION MASS SPECTROMETRY. Further, adapter **111** with electrical contact spring **112** is fitted over port **109**. Nanospray assembly **90** is inserted through adapter **111** and port **109** until finally coming into contact with and fitting over capillary section **233**. At this point o-ring **100** forms a seal between capillary section **233** and union **99**. In this way multiple part capillary **235** is formed from capillary sections **98** and **233** in accordance with copending application METHOD AND APPARATUS FOR A MULTIPLE PART CAPILLARY DEVICE FOR USE IN MASS SPECTROMETRY. Notice that assembly **90** can be inserted and extracted from spray chamber **240**, without tools, by simply pushing and pulling respectively assembly **90** through port **109** along axis **106**.

[0064] When inserted into spray chamber **240**, nanospray assembly **90** is supported on one end by adapter **111** and port **109** and is supported on the other end by capillary **233**. In the preferred embodiment, cover **107** is electrically grounded by contact with the rest of the source (not shown).

Adapter **111** is grounded by contact with cover **107**. And base **91**—together with union **94**, spray needle **93**, and retainer **96**—is grounded by contact with adapter **111** via spring contact **112**. Capillary section **98** together with cap **97** and union **99** are held at a high potential via metal coating **30A** on capillary section **233**.

[0065] Depicted in **FIG. 10** is nanospray assembly **90** as it is inserted into spray chamber **240** of a complete ionization source designed according to co-pending application IONIZATION SOURCE FOR MASS SPECTROMETRY. During normal operation of preferred embodiment nanospray assembly **90**, sample solution is formed into droplets at atmospheric pressure by spraying the sample solution from spray needle **93** into spray chamber **240**. The spray is induced by the application of a high potential between spray needle **93** and entrance cap **97** within spray chamber **240**. Sample droplets from the spray evaporate while in spray chamber **240** thereby leaving behind an ionized sample material (i.e., sample ions). These sample ions are accelerated toward capillary inlet **126** of capillary section **98** by the electric field between spray needle **93**, entrance cap **97** and inlet **126** of first section **98** of capillary **235** and by the flow of gas towards and into inlet **126**. The design of entrance cap **97** provides the additional advantage over prior art nanospray devices that the gas flow through hole **105** tends to focus ions into inlet **126**. That is, gas flow in the nanospray assembly according to the present invention is well controlled. All gas entering channel **113** must flow through hole **105**. Because needle tip **104** is inserted into hole **105** for normal operation, ions produced at tip **104** are immediately entrained in the gas flow and transported to and through channel **113**. As a result, the position of spray needle **93** within the assembly is again less critical than in prior art devices.

[0066] The ions are transported through first channel **113** into and through second channel **232** to capillary outlet **234**. As described above first section **98** is joined to second section **233** in a sealed manner by union **99**. The flow of gas created by the pressure differential between spray chamber **240** and first transfer region **245** further causes ions to flow through the capillary channels from the spray chamber toward exit elements **255** and the mass analyzer (not shown).

[0067] Still referring to **FIG. 9**, first transfer region **245** is formed by mounting flange **248** on source block **254** where a vacuum tight seal is formed between flange **248** and source block **254** by o-ring **258**. Capillary **235** penetrates through a hole in flange **248** where another vacuum tight seal is maintained (i.e., between flange **248** and capillary **235**) by o-ring **256**. A vacuum is then generated and maintained in first transfer **245** by a pump (e.g., a roughing pump, etc., not shown). The inner diameter and length of capillary **235** and the pumping speed of the pump are selected to provide as high a rate of gas flow through capillary **235** as reasonably possible while maintaining a pressure of 1 mbar in the first transfer region **245**. A higher gas flow rate through capillary **235** will result in more efficient transport of ions.

[0068] Next, as further shown in **FIG. 9**, first skimmer **251** is placed adjacent to capillary exit **234** within first transfer region **245**. An electric potential between capillary outlet end **234** and first skimmer **251** accelerates the sample ions toward first skimmer **251**. A fraction of the sample ions then pass through an opening in first skimmer **251** and into

second pumping region **243** where pre-hexapole **249** is positioned to guide the sample ions from the first skimmer **251** to second skimmer **252**. Second pumping region **243** is pumped to a lower pressure than first transfer region **245** by pump **253**. Again, a fraction of the sample ions pass through an opening in second skimmer **252** and into third pumping region **244**, which is pumped to a lower pressure than second pumping region **243** via pump **253**.

[0069] Once in third pumping region **244**, the sample ions are guided from second skimmer **252** to exit electrodes **255** by hexapole **250**. While in hexapole **250** ions undergo collisions with a gas (i.e., a collisional gas) and are thereby cooled to thermal velocities. The ions then reach exit electrodes **255** and are accelerated from the ionization source into the mass analyzer (not shown) for subsequent analysis.

[0070] Referring lastly to FIGS. 11A-C, shown is yet another alternative embodiment of a spray needle according to the invention, wherein spray needle **131** further comprises a multiple element tip (or "multi-tip"). As shown, spray needle **131**, similar to the preferred embodiment of the invention shown in FIGS. 5A-C, comprises two component parts, support **130** and foil **133**. Support **130** is preferably constructed from a rigid and electrically conductive material (e.g., steel, etc.). It is also preferred that the support **30** be a solid yet thin structure (i.e., on the order of 400 μm or less in thickness). The thickness of the support contributes to the determination of the loading and spray properties of the sprayer (i.e., how fast the solution will flow into the sprayer, the potential at which the sprayer must be operated, the optimal distance between the sprayer and ESI orifice, and the solution flow rate during spray etc.), because the thickness of support **130** determines the size of foil **133**. It is further preferred, as shown in FIG. 11B, that support **130** have a rectangular cross section. This geometry eases the elimination of voids or bubbles which interfere with the spray of the solution. However, support **30** may have a different cross-sectional shape (e.g., triangular, circular, hexagonal, etc.). Such change in the shape of support **130**, however, may alter the spray properties of the sprayer. Thus, different structures may be ideal for different sample solutions.

[0071] Generally, foil **133** may be constructed using a piece of electrically conducting "foil" which is cut at an angle α , as shown in FIG. 11A. In this embodiment, foil **133** is attached to the outer surface of support **130** at one end of support **130**, as depicted in FIGS. 11A and 11C. Foil **133** is attached such that it is in electrical contact with support **130**. Preferably, an adhesive is used to attach foil **133** to support **130**, but other means for attaching foil **133** to support **130** may be used, such as soldering, etc.

[0072] Foil **133** is preferably constructed from a chemically inert and easily cleaned material (e.g., gold, copper, platinum, stainless steel (because of its limited reactivity to certain compounds), etc.). For example, certain species are not readily protonated, but will accept, for example, silver or copper ions as adducts. Therefore, use of such different materials for foil **133** may alter the life and spray properties of the spray needle **131**, as described above with respect to the preferred embodiment. Of course, other materials might be used in the construction of foil **133**, depending on the particular electrochemical or reactive properties desired (e.g., the use of copper instead of gold for foil **133** may result

in the formation of copper ions, thus having the potential for forming complexes with analyte species) in order to enhance signal intensity in certain analyses.

[0073] As described above for the preferred embodiment, it is preferred that foil **133** be constructed from a very thin piece of metal (i.e., about 100 μm in thickness). However, the thickness, particular metal, etc., used for foil **133** may be chosen based on the desired properties (i.e., durability, formation, spray type, etc.).

[0074] Importantly, spray needle **131** according to this alternate embodiment of the invention, as shown in FIGS. 11A-C, comprises tip **132** which, as previously described, may be formed by wrapping or folding a portion of foil **133** around one end of support **130** and affixing foil **133** thereto. Once wrapped or folded, the exposed end of foil **133** is preferably cut at an angle α **134** as shown in FIG. 11A, thereby forming tip **132**. In addition, tip **132** may have a plurality of (i.e., 26, 50, 100, etc.) extremely fine elements **136** (i.e., on the order of 50 μm or less) extending slightly therefrom. Preferably, these fine elements **136** are individual elements positioned lengthwise within foil **133**, as shown in FIG. 11C. During use of such spray needle **131**, the sample solution is sprayed from each of these individual fine elements **136**, thereby resulting in a very fine spray of sample solution, which minimizes the amount of solution lost (i.e., not introduced into the analyzer). Alternatively, tip **132** may be designed such that it comprises a plurality of tips, rather than the additional fine elements **136** being positioned within foil **133**. Alternatively, the individual fine elements **136** may be incorporated into the embodiments depicted in FIGS. 6A-C & 7A-C in a manner similar to that shown and described for FIGS. 11A-C.

[0075] While the present invention has been described with reference to one or more preferred embodiments, such embodiments are merely exemplary and are not intended to be limiting or represent an exhaustive enumeration of all aspects of the invention. The scope of the invention, therefore, shall be defined solely by the following claims. Further, it will be apparent to those of skill in the art that numerous changes may be made in such details without departing from the spirit and the principles of the invention. It should be appreciated that the present invention is capable of being embodied in other forms without departing from its essential characteristics.

What is claimed is:

1. An apparatus for the introduction of sample into a mass analyzer, comprising:

- a first component having a first end and a second end; and
- a second component having a longitudinal bore there-through;

wherein said second component is attached to said second end of said first component such that said first component and said longitudinal bore of said second component are coaxial.

2. An apparatus according to claim 1, wherein said second component has first and second surfaces, and wherein said first surface of said second component is affixed to said first component at said second end.

3. An apparatus according to claim 1, wherein said second component comprises an electrically conducting foil.

4. An apparatus according to claim 1, wherein said second component is thin.

5. An apparatus according to claim 1, wherein said second component has a width of approximately 100 microns.

6. An apparatus according to claim 1, wherein said second component is constructed from a chemically inert material.

7. An apparatus according to claim 6, wherein said chemically inert material is selected from the group consisting of gold, platinum and stainless steel.

8. An apparatus according to claim 1, wherein said second component is shaped and positioned such that said longitudinal bore is tapered from a first end thereof to a second end thereof.

9. An apparatus according to claim 1, wherein said first component comprises a rigid material.

10. An apparatus according to claim 1, wherein said first component comprises an electrically conductive material.

11. An apparatus according to claim 10, wherein said material is steel.

12. An apparatus according to claim 1, wherein said first component has a thickness of approximately equal to or less than 400 microns.

13. An apparatus according to claim 1, wherein said first component has a rectangular cross section.

14. An apparatus according to claim 1, wherein said first component has a circular cross section.

15. An apparatus according to claim 1, wherein said first component has a triangular cross section.

16. An apparatus according to claim 1, wherein said second component is cut at an angle α to said longitudinal bore therethrough.

17. An apparatus according to claim 16, such that said angle α is within the range of 0 to 90 degrees.

18. An apparatus according to claim 16, such that said angle α is within the range of 30 to 60 degrees.

19. An apparatus according to claim 1, wherein said second component comprises a proximal end and a distal end.

20. An apparatus according to claim 19, wherein said proximal end is attached to said second end of said first component.

21. An apparatus according to claim 19, wherein said distal end is constructed by cutting said second component at an angle α to said longitudinal bore therethrough.

22. An apparatus according to claim 21, such that said angle α is within the range of 0 to 90 degrees.

23. An apparatus according to claim 21, such that said angle α is within the range of 30 to 60 degrees.

24. An apparatus according to claim 19, wherein said distal end is narrower than said proximal end.

25. An apparatus according to claim 19, wherein said distal end has a width of approximately 200 microns.

26. An apparatus according to claim 19, wherein said distal end has a width in the range of approximately 20 to 50 microns.

27. An apparatus according to claim 19, wherein said opening has a width of approximately 5 microns.

28. An apparatus according to claim 19, wherein said distal end culminates in an angled point tip.

29. An apparatus according to claim 19, wherein said distal end culminates in a circular tip.

30. An apparatus according to claim 19, wherein sample is introduced from said spray needle into said mass analyzer at said distal end.

31. An apparatus according to claim 1, wherein said second component is coated with a polymer.

32. An apparatus for the introduction of sample into a mass analyzer, said apparatus comprising a needle having first and second ends, wherein said needle has an aperture along its length, parallel to the axis of said needle extending from said second end toward said first end.

33. An apparatus according to claim 32, wherein said needle comprises a rigid material.

34. An apparatus according to claim 32, wherein said needle comprises an electrically conductive material.

35. An apparatus according to claim 32, wherein said needle has a thickness of approximately 400 microns.

36. An apparatus according to claim 32, wherein said needle has a circular cross section.

37. An apparatus according to claim 32, wherein said first end culminates in a tip.

38. An apparatus according to claim 37, wherein said tip comprises a hole.

39. An apparatus according to claim 38, wherein said hole is approximately 200 microns in diameter.

40. An apparatus according to claim 38, wherein said hole has a diameter in the range of approximately 20 to 50 microns.

41. An apparatus according to claim 38, wherein said hole has a diameter of approximately 5 microns.

42. An apparatus according to claim 32, wherein said second end culminates in an opening.

43. An apparatus according to claim 32, wherein sample is introduced from said needle into said mass analyzer at said first end.

44. An apparatus for the introduction of sample into a mass analyzer, said apparatus comprising a needle having first and second ends, wherein said needle has a plurality of apertures along its length, aligned parallel to said axis of said needle extending from said second end towards said first end.

45. An apparatus according to claim 44, wherein said needle comprises a rigid material.

46. An apparatus according to claim 44, wherein said needle comprises an electrically conductive material.

47. An apparatus according to claim 44, wherein said needle has a thickness of approximately 400 microns.

48. An apparatus according to claim 44, wherein said needle has a circular cross section.

49. An apparatus according to claim 44, wherein said first end culminates in a tip.

50. An apparatus according to claim 49, wherein said tip comprises a hole.

51. An apparatus according to claim 50, wherein said hole is approximately 200 microns in diameter.

52. An apparatus according to claim 50, wherein said hole has a diameter in the range of approximately 20 to 50 microns.

53. An apparatus according to claim 50, wherein said hole has a diameter of approximately 5 microns.

54. An apparatus according to claim 44, wherein said second end culminates in an opening.

55. An apparatus according to claim 44, wherein sample is introduced from said needle into said mass analyzer at said first end.

56. An apparatus for the introduction of sample into a mass analyzer, comprising:

a first component having a first end and a second end;

a second component having a longitudinal bore there-through; and

a plurality of fine elements;

wherein said second component is attached to said second end of said first component such that said first component and said longitudinal bore of said second component are coaxial, and wherein said plurality of elements are positioned within said longitudinal bore of said second component such that said elements extend therefrom.

57. An apparatus according to claim 56, wherein said second component has first and second surfaces, and wherein said first surface of said second component is affixed to said first component at said second end.

58. An apparatus according to claim 56, wherein said second component comprises an electrically conducting foil.

59. An apparatus according to claim 56, wherein said second component is thin.

60. An apparatus according to claim 56, wherein said second component has a width of approximately 100 microns.

61. An apparatus according to claim 56, wherein said second component is constructed from a chemically inert material.

62. An apparatus according to claim 61, wherein said chemically inert material is selected from the group consisting of gold, platinum and stainless steel.

63. An apparatus according to claim 56, wherein said second component is shaped and positioned such that said longitudinal bore is tapered from a first end thereof to a second end thereof.

64. An apparatus according to claim 56, wherein said first component comprises a rigid material.

65. An apparatus according to claim 56, wherein said first component comprises an electrically conductive material.

66. An apparatus according to claim 65, wherein said material is steel.

67. An apparatus according to claim 56, wherein said first component has a thickness of approximately equal to or less than 400 microns.

68. An apparatus according to claim 56, wherein said first component has a rectangular cross section.

69. An apparatus according to claim 56, wherein said first component has a circular cross section.

70. An apparatus according to claim 56, wherein said first component has a triangular cross section.

71. An apparatus according to claim 56, wherein said second component is cut at an angle α to said longitudinal bore therethrough.

72. An apparatus according to claim 71, such that said angle α is within the range of 0 to 90 degrees.

72. An apparatus according to claim 71, such that said angle α is within the range of 30 to 60 degrees.

73. An apparatus according to claim 56, wherein said second component comprises a proximal end and a distal end.

74. An apparatus according to claim 73, wherein said proximal end is attached to said second end of said first component.

75. An apparatus according to claim 73, wherein said distal end is constructed by cutting said second component at an angle α to said longitudinal bore therethrough.

76. An apparatus according to claim 75, such that said angle α is within the range of 0 to 90 degrees.

77. An apparatus according to claim 75, such that said angle α is within the range of 30 to 60 degrees.

78. An apparatus according to claim 73, wherein said distal end is narrower than said proximal end.

79. An apparatus according to claim 73, wherein said distal end has a width of approximately 200 microns.

80. An apparatus according to claim 73, wherein said distal end has a width in the range of approximately 20 to 50 microns.

81. An apparatus according to claim 73, wherein said opening has a width of approximately 5 microns.

82. An apparatus according to claim 73, wherein said distal end culminates in an angled point tip.

83. An apparatus according to claim 74, wherein said distal end culminates in a circular tip.

84. An apparatus according to claim 73, wherein sample is introduced from said spray needle into said mass analyzer at said distal end.

85. An apparatus according to claim 56, wherein said second component is coated with a polymer.

* * * * *