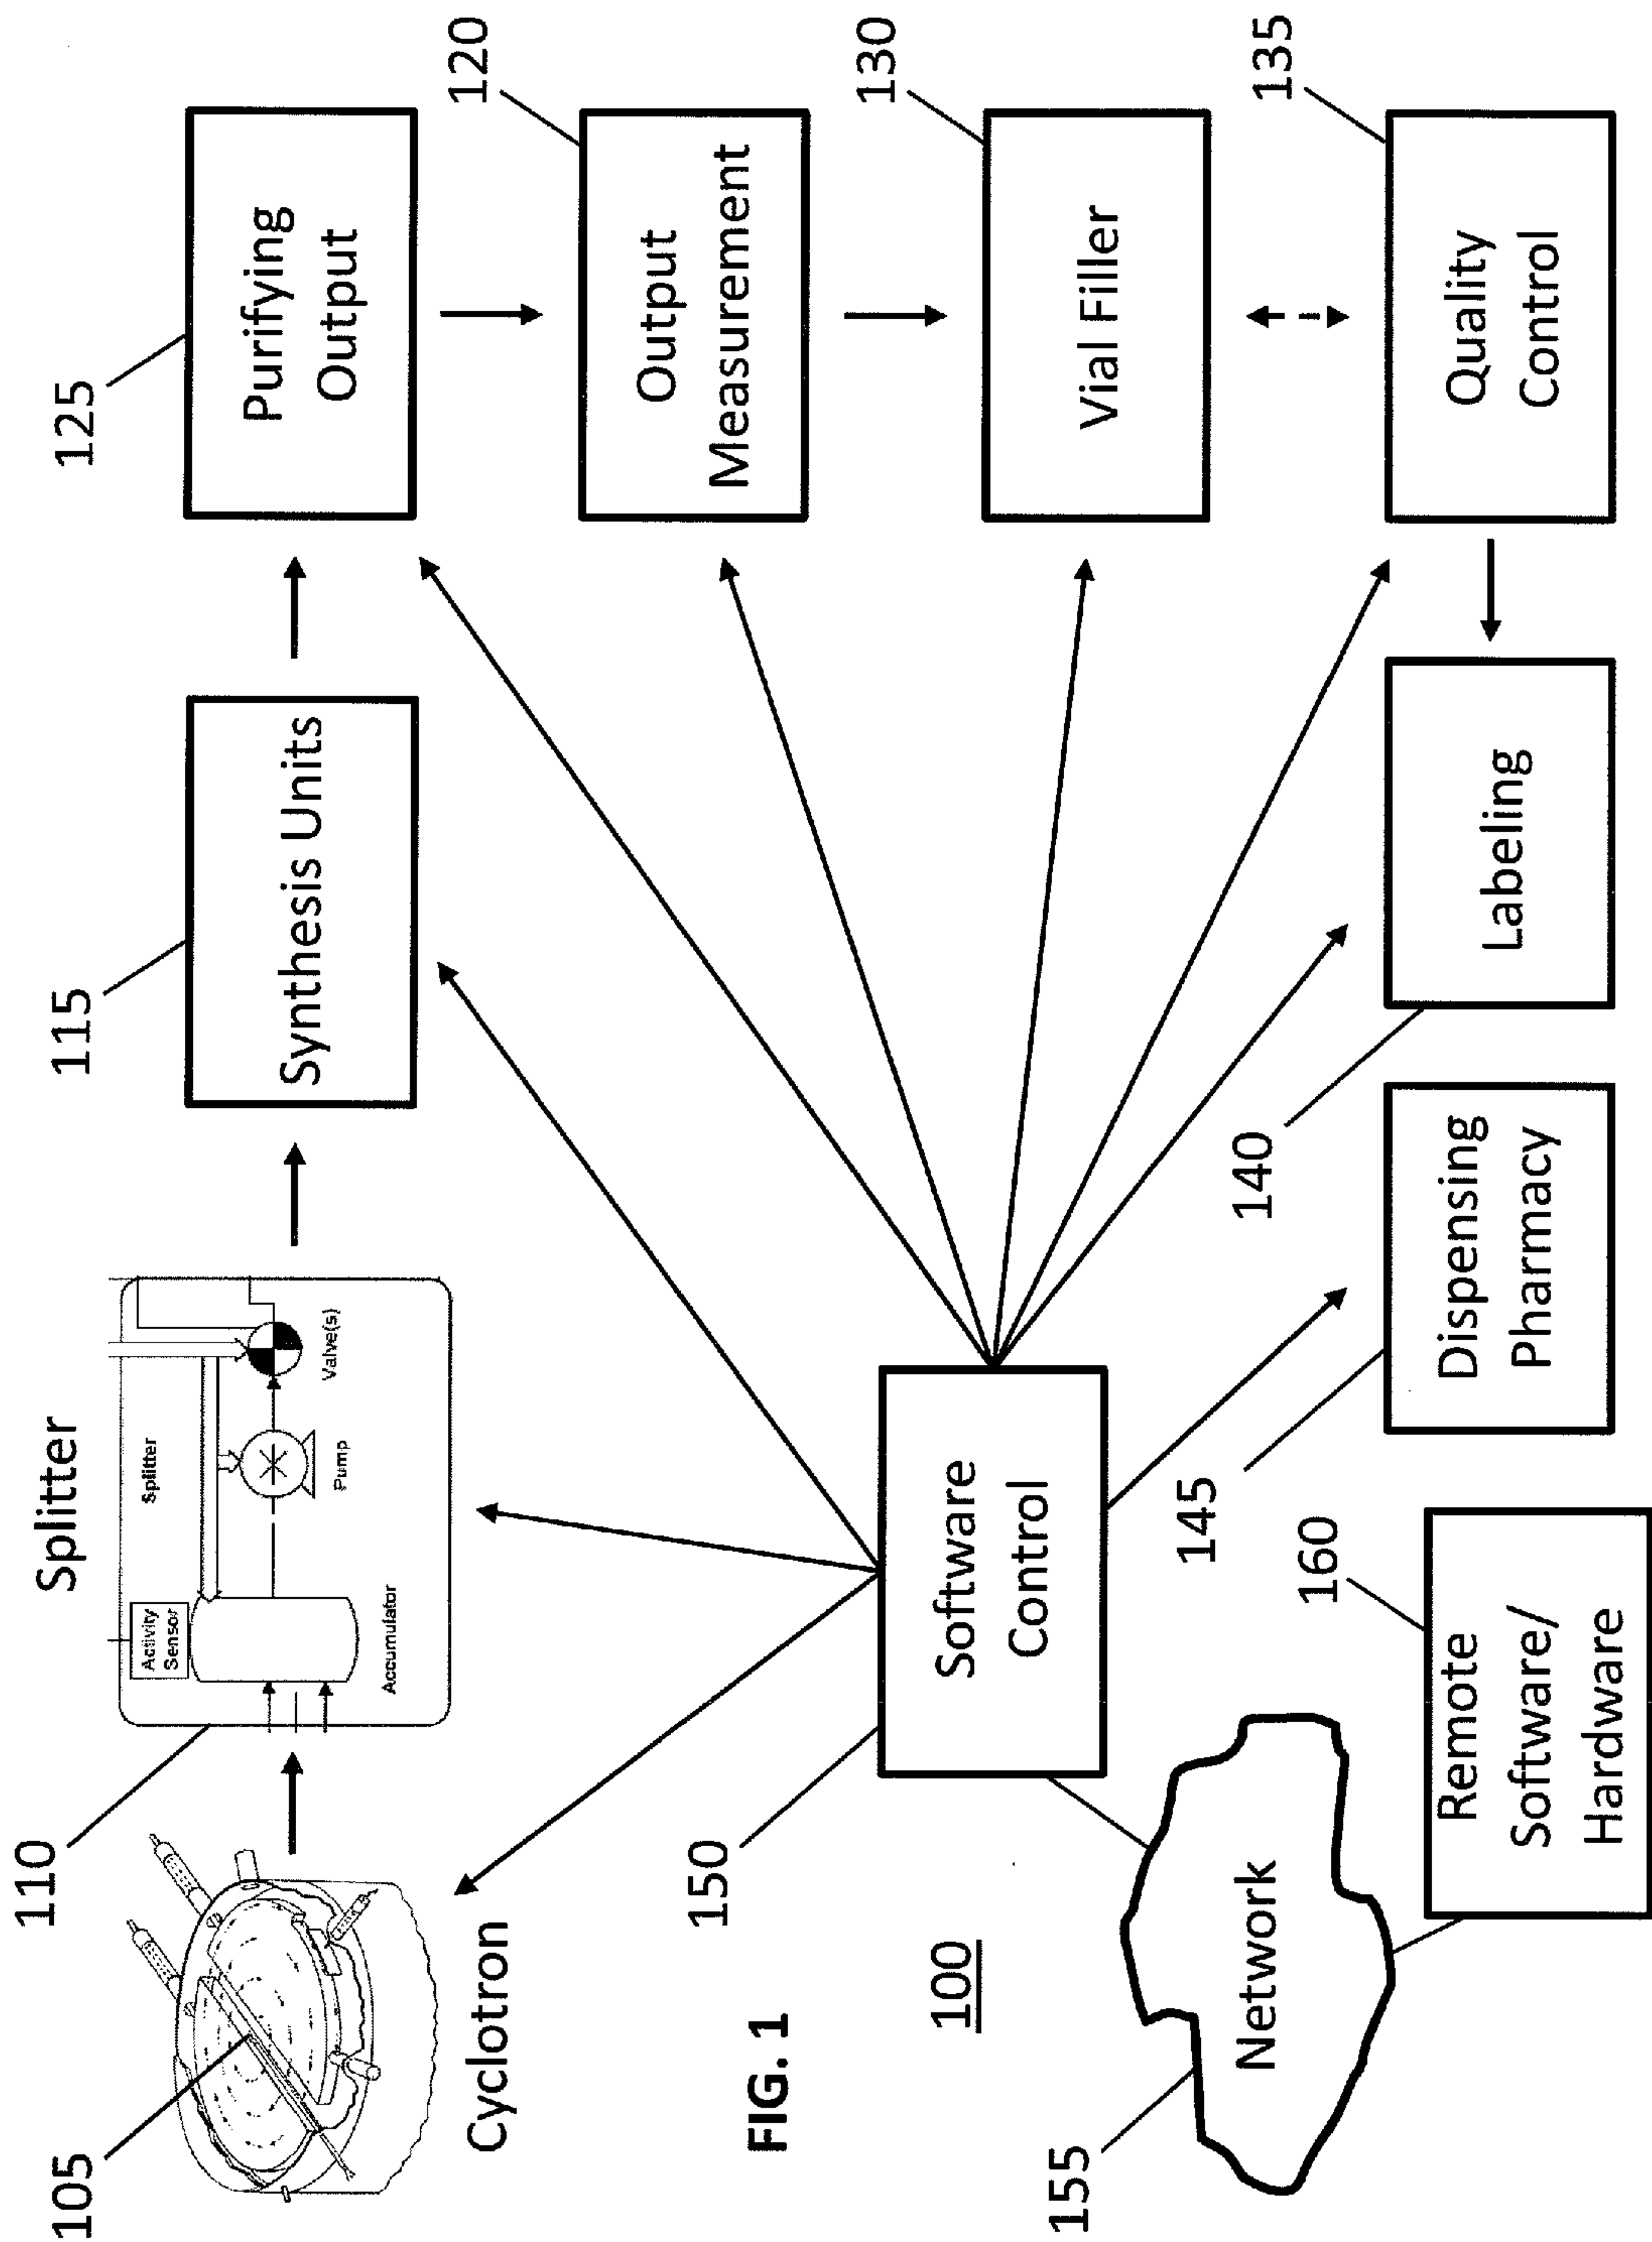


US 20130102772A1

(19) **United States**(12) **Patent Application Publication**  
**ESHIMA et al.**(10) **Pub. No.: US 2013/0102772 A1**(43) **Pub. Date: Apr. 25, 2013**(54) **SYSTEMS, METHODS AND DEVICES FOR  
PRODUCING, MANUFACTURING AND  
CONTROL OF  
RADIOPHARMACEUTICALS-FULL**(75) Inventors: **Dennis ESHIMA**, Phoenix, AZ (US);  
**Mehmet Husnu**, Phoenix, AZ (US); **Jim  
Stone**, Alpharetta, GA (US); **Derrick  
Alcaide**, Los Angeles, CA (US); **Henry  
Padgett**, Dublin, OH (US); **Joseph E.  
Zambanini**, Delaware, OH (US);  
**Thomas A. Klausning**, Powell, OH (US);  
**Chad E. Bouton**, Powell, OH (US);  
**Brian C. Kelley**, Pataskala, OH (US);  
**Scott N. Danhof**, Plain City, OH (US);  
**David A. Holley**, Lancaster, OH (US);  
**Jeffrey T. Stroup**, Upper Arlington, OH  
(US); **James B. Gleeson**, Columbus, OH  
(US); **Eric Hassenpflug**, Westerville,  
OH (US); **James A. Prescott**, Columbus,  
OH (US); **Herman Benecke**, Columbus,  
OH (US); **Daniel B. Garbark**,  
Blacklick, OH (US)(73) Assignee: **CARDINAL HEALTH 414, LLC**,  
Dublin, OH (US)(21) Appl. No.: **13/550,425**(22) Filed: **Jul. 16, 2012****Related U.S. Application Data**(60) Provisional application No. 61/508,294, filed on Jul.  
15, 2011, provisional application No. 61/508,383,  
filed on Jul. 15, 2011, provisional application No.  
61/508,374, filed on Jul. 15, 2011, provisional appli-  
cation No. 61/508,382, filed on Jul. 15, 2011, provi-  
sional application No. 61/508,402, filed on Jul. 15,  
2011, provisional application No. 61/508,394, filed on  
Jul. 15, 2011, provisional application No. 61/508,359,  
filed on Jul. 15, 2011, provisional application No.  
61/508,367, filed on Jul. 15, 2011, provisional appli-  
cation No. 61/508,382, filed on Jul. 15, 2011, provi-sional application No. 61/508,464, filed on Jul. 15,  
2011, provisional application No. 61/508,353, filed on  
Jul. 15, 2011, provisional application No. 61/508,408,  
filed on Jul. 15, 2011, provisional application No.  
61/508,349, filed on Jul. 15, 2011, provisional appli-  
cation No. 61/508,409, filed on Jul. 15, 2011, provi-  
sional application No. 61/553,029, filed on Oct. 28,  
2011.**Publication Classification**(51) **Int. Cl.**  
**B01J 19/00** (2006.01)  
**B65B 1/00** (2006.01)  
(52) **U.S. Cl.**  
CPC ..... **B01J 19/0006** (2013.01); **B65B 1/00**  
(2013.01)  
USPC ..... **536/28.2**; 536/122; 548/327.5; 422/159;  
422/119; 422/110; 53/473(57) **ABSTRACT**

Systems, methods, and devices for generating radionuclides for use in production of radiopharmaceuticals; synthesizing the radionuclides generated and removing any unwanted products; measuring the quantity and activity level of the synthesized radionuclides; distributively delivering the radionuclides in appropriate quantities to modular cassette synthesis units in a modular cassette subsystem for contemporaneous/parallel production of radiopharmaceutical output and that allow reuse and/or quick, safe, and disposable replacement of portions of the subsystem; delivering non-radionuclide components to the modular cassette synthesis units as part of production of radiopharmaceutical output; measuring the quantity and activity level of each stream of radiopharmaceutical output; purifying the radiopharmaceutical output; dispensing individual doses in sterile vial(s); automatically producing labeling and dose related information; performing automated quality control on extracted samples of produced radiopharmaceutical output; and providing software and hardware controls for overall and sub-portion operation for optional remote data collection, communication, and/or control.






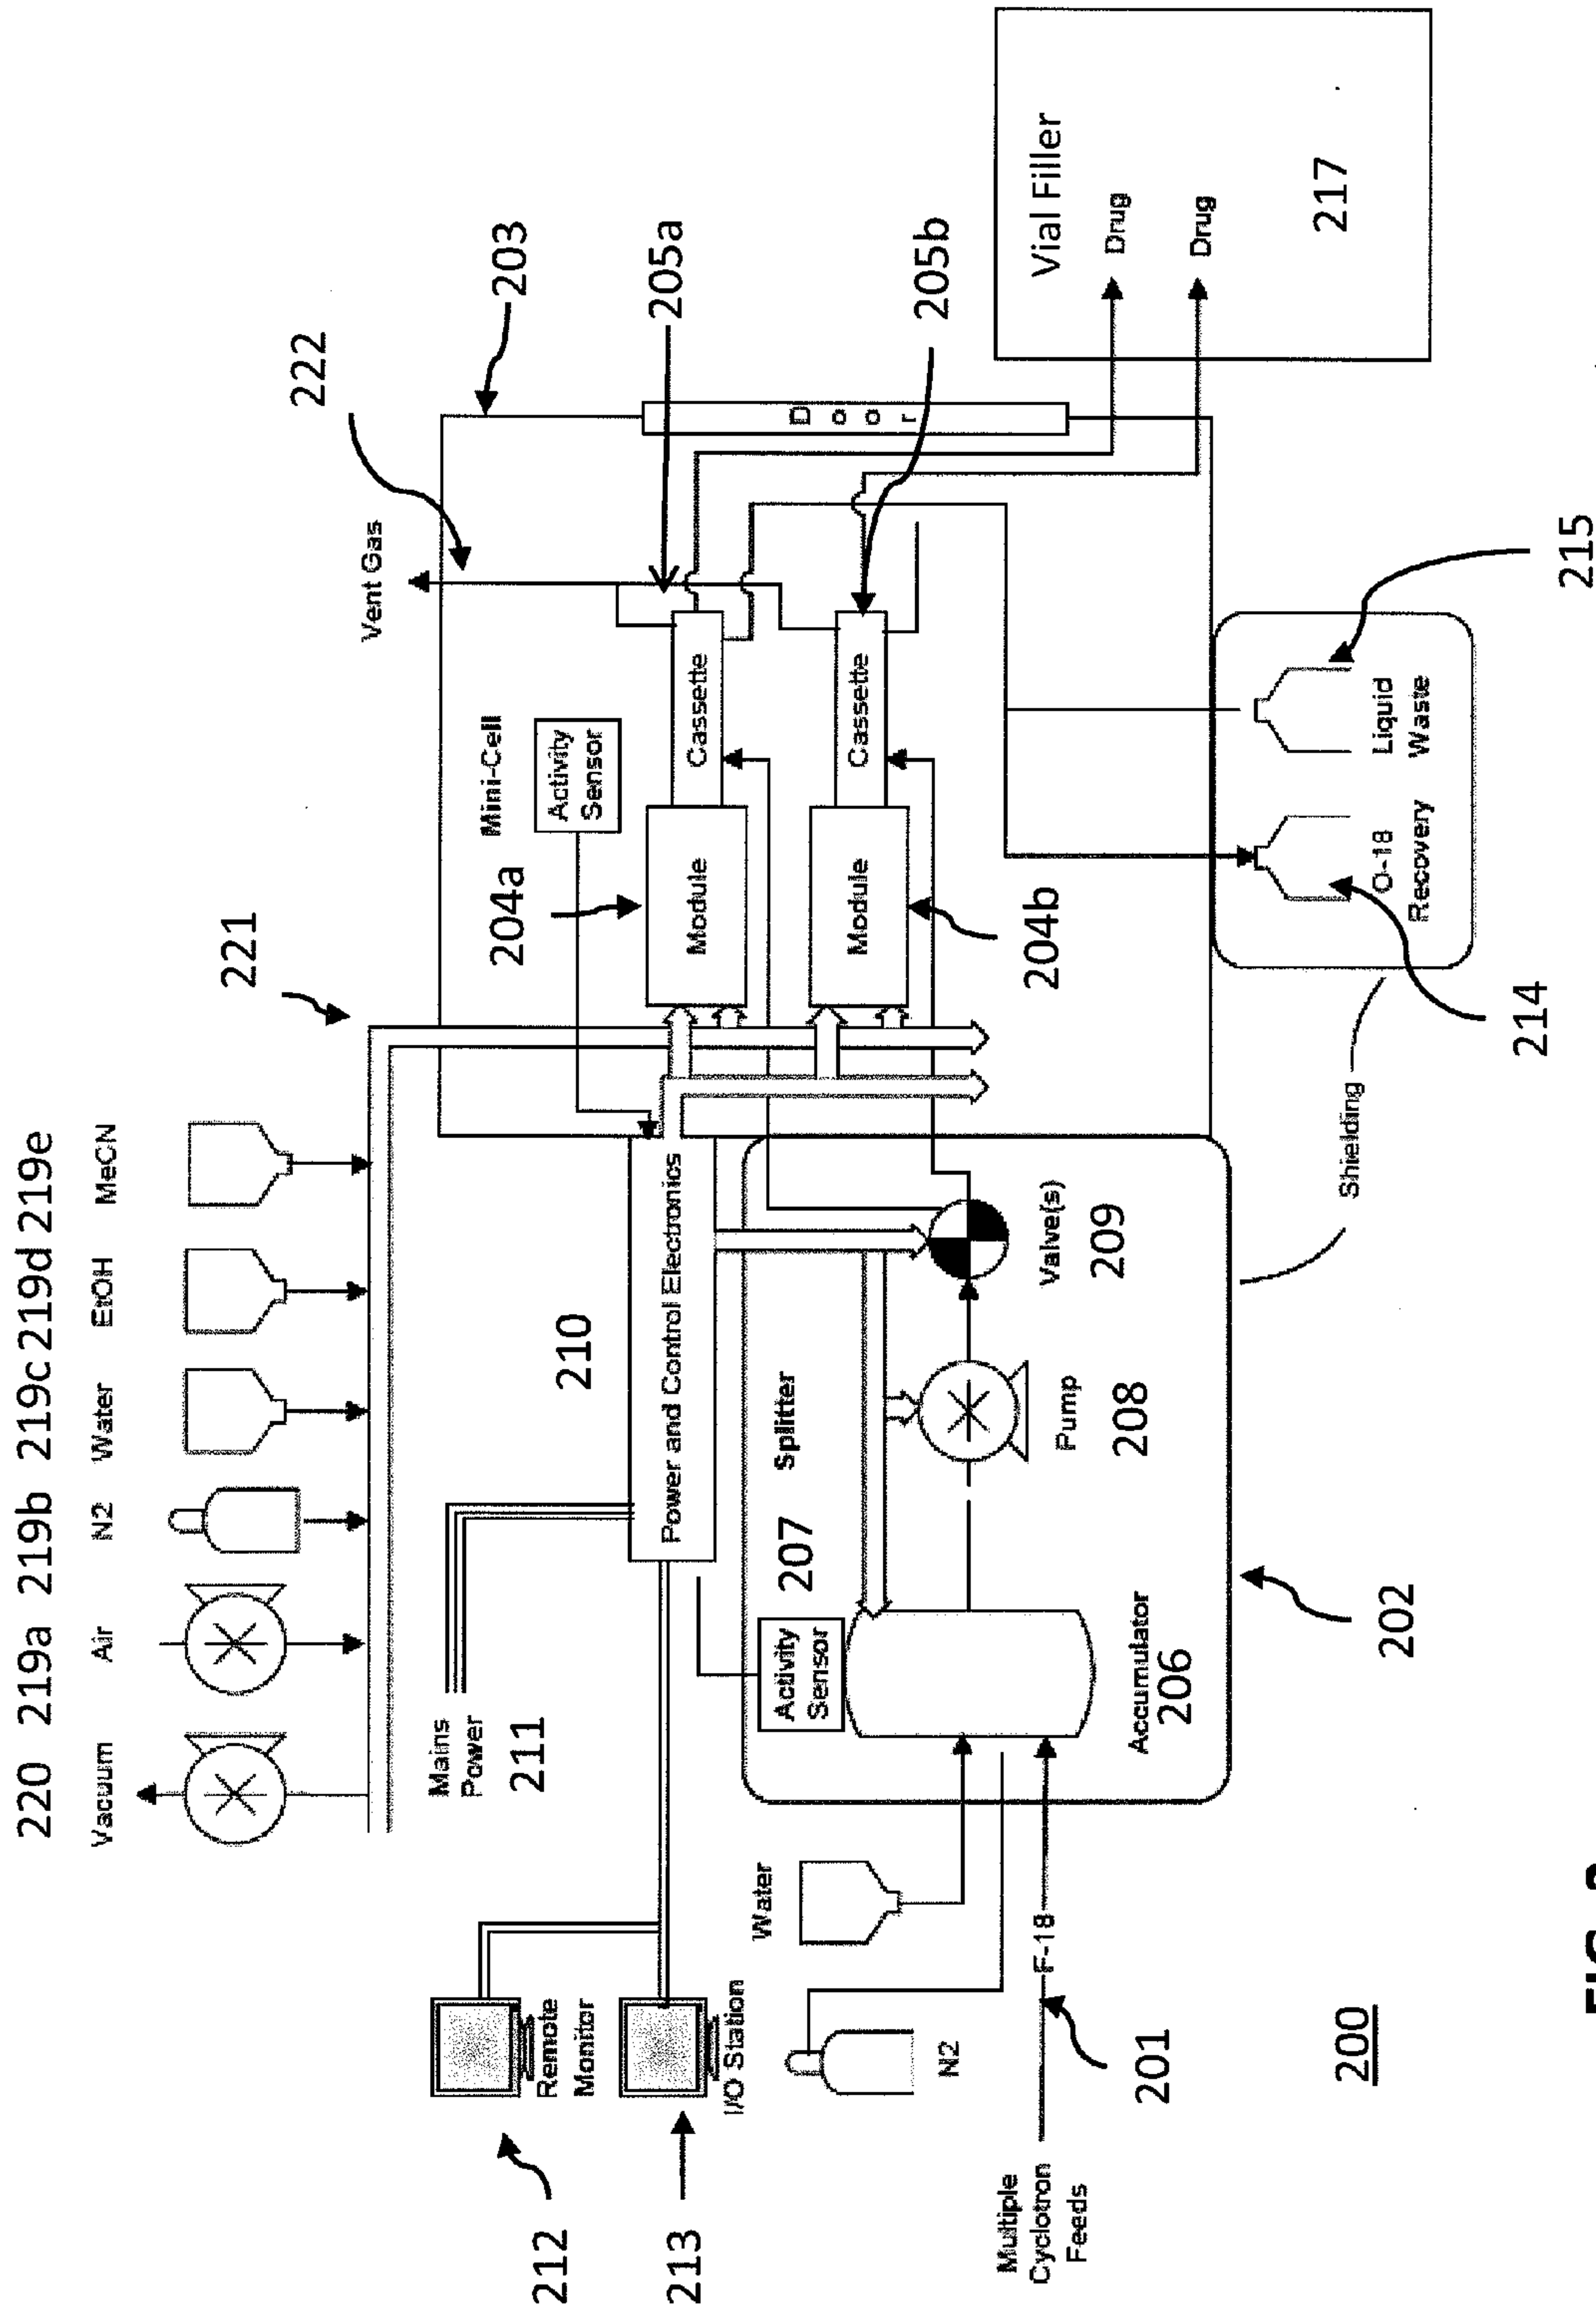


FIG. 2

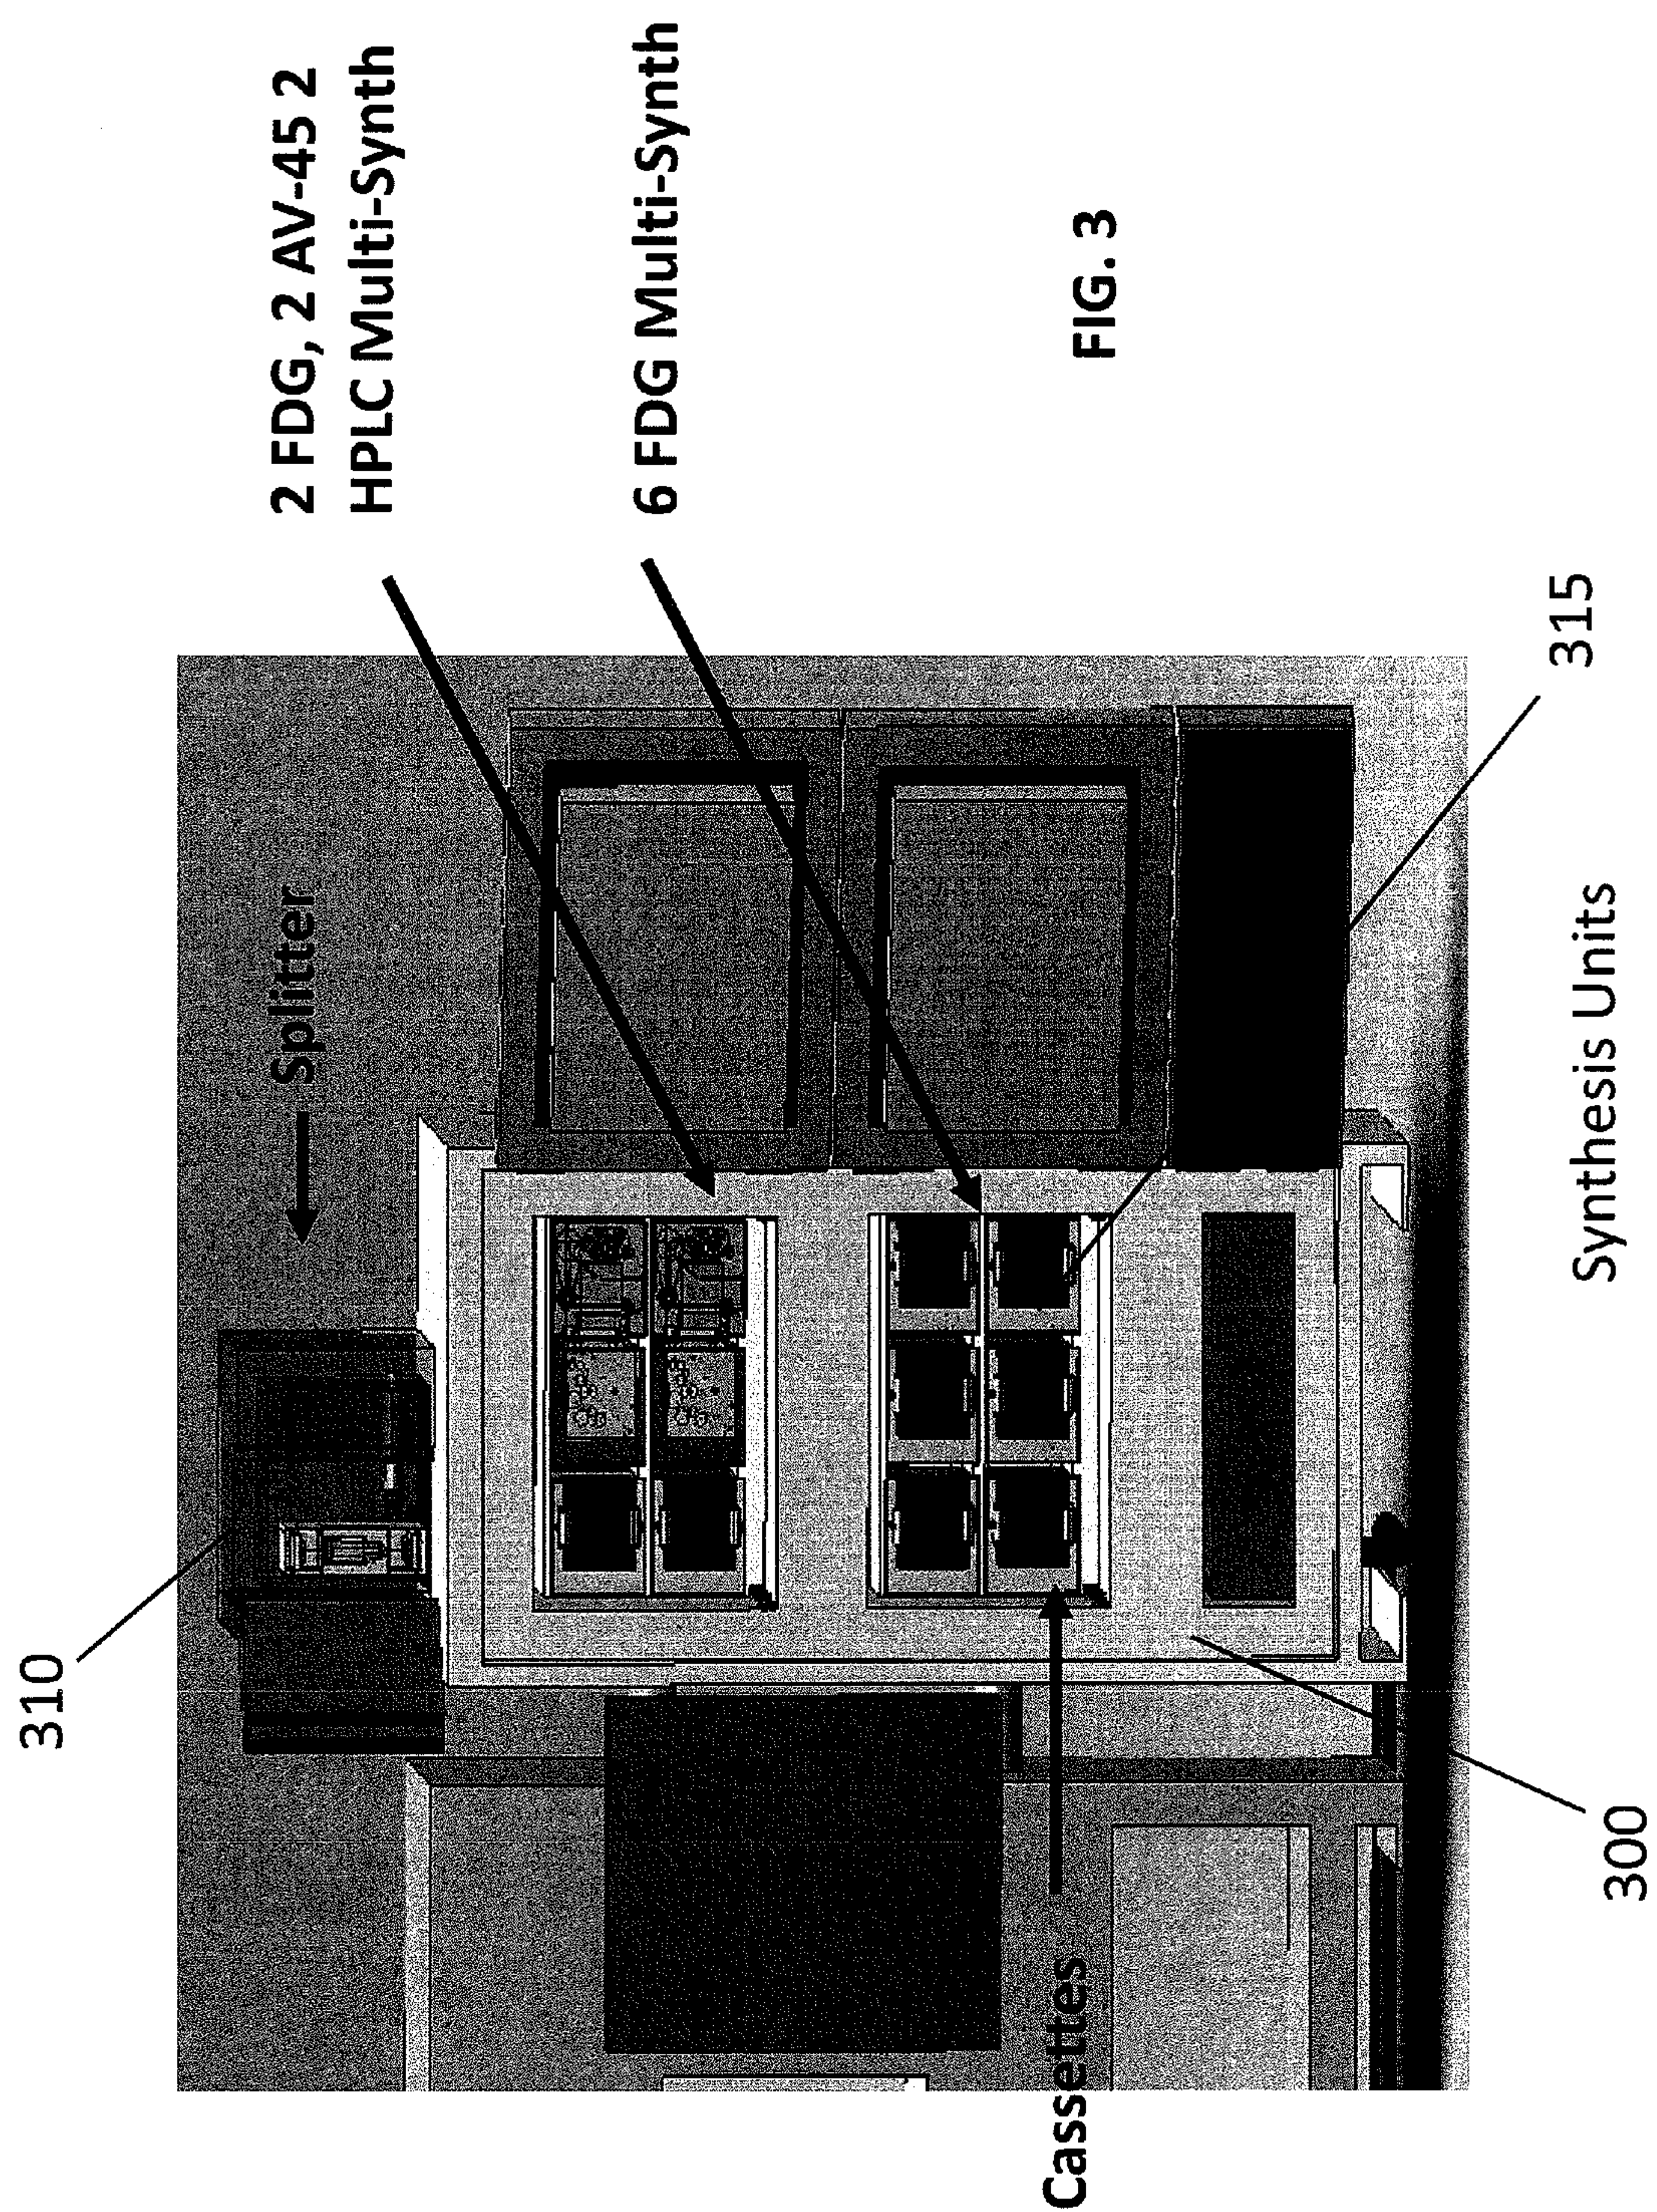

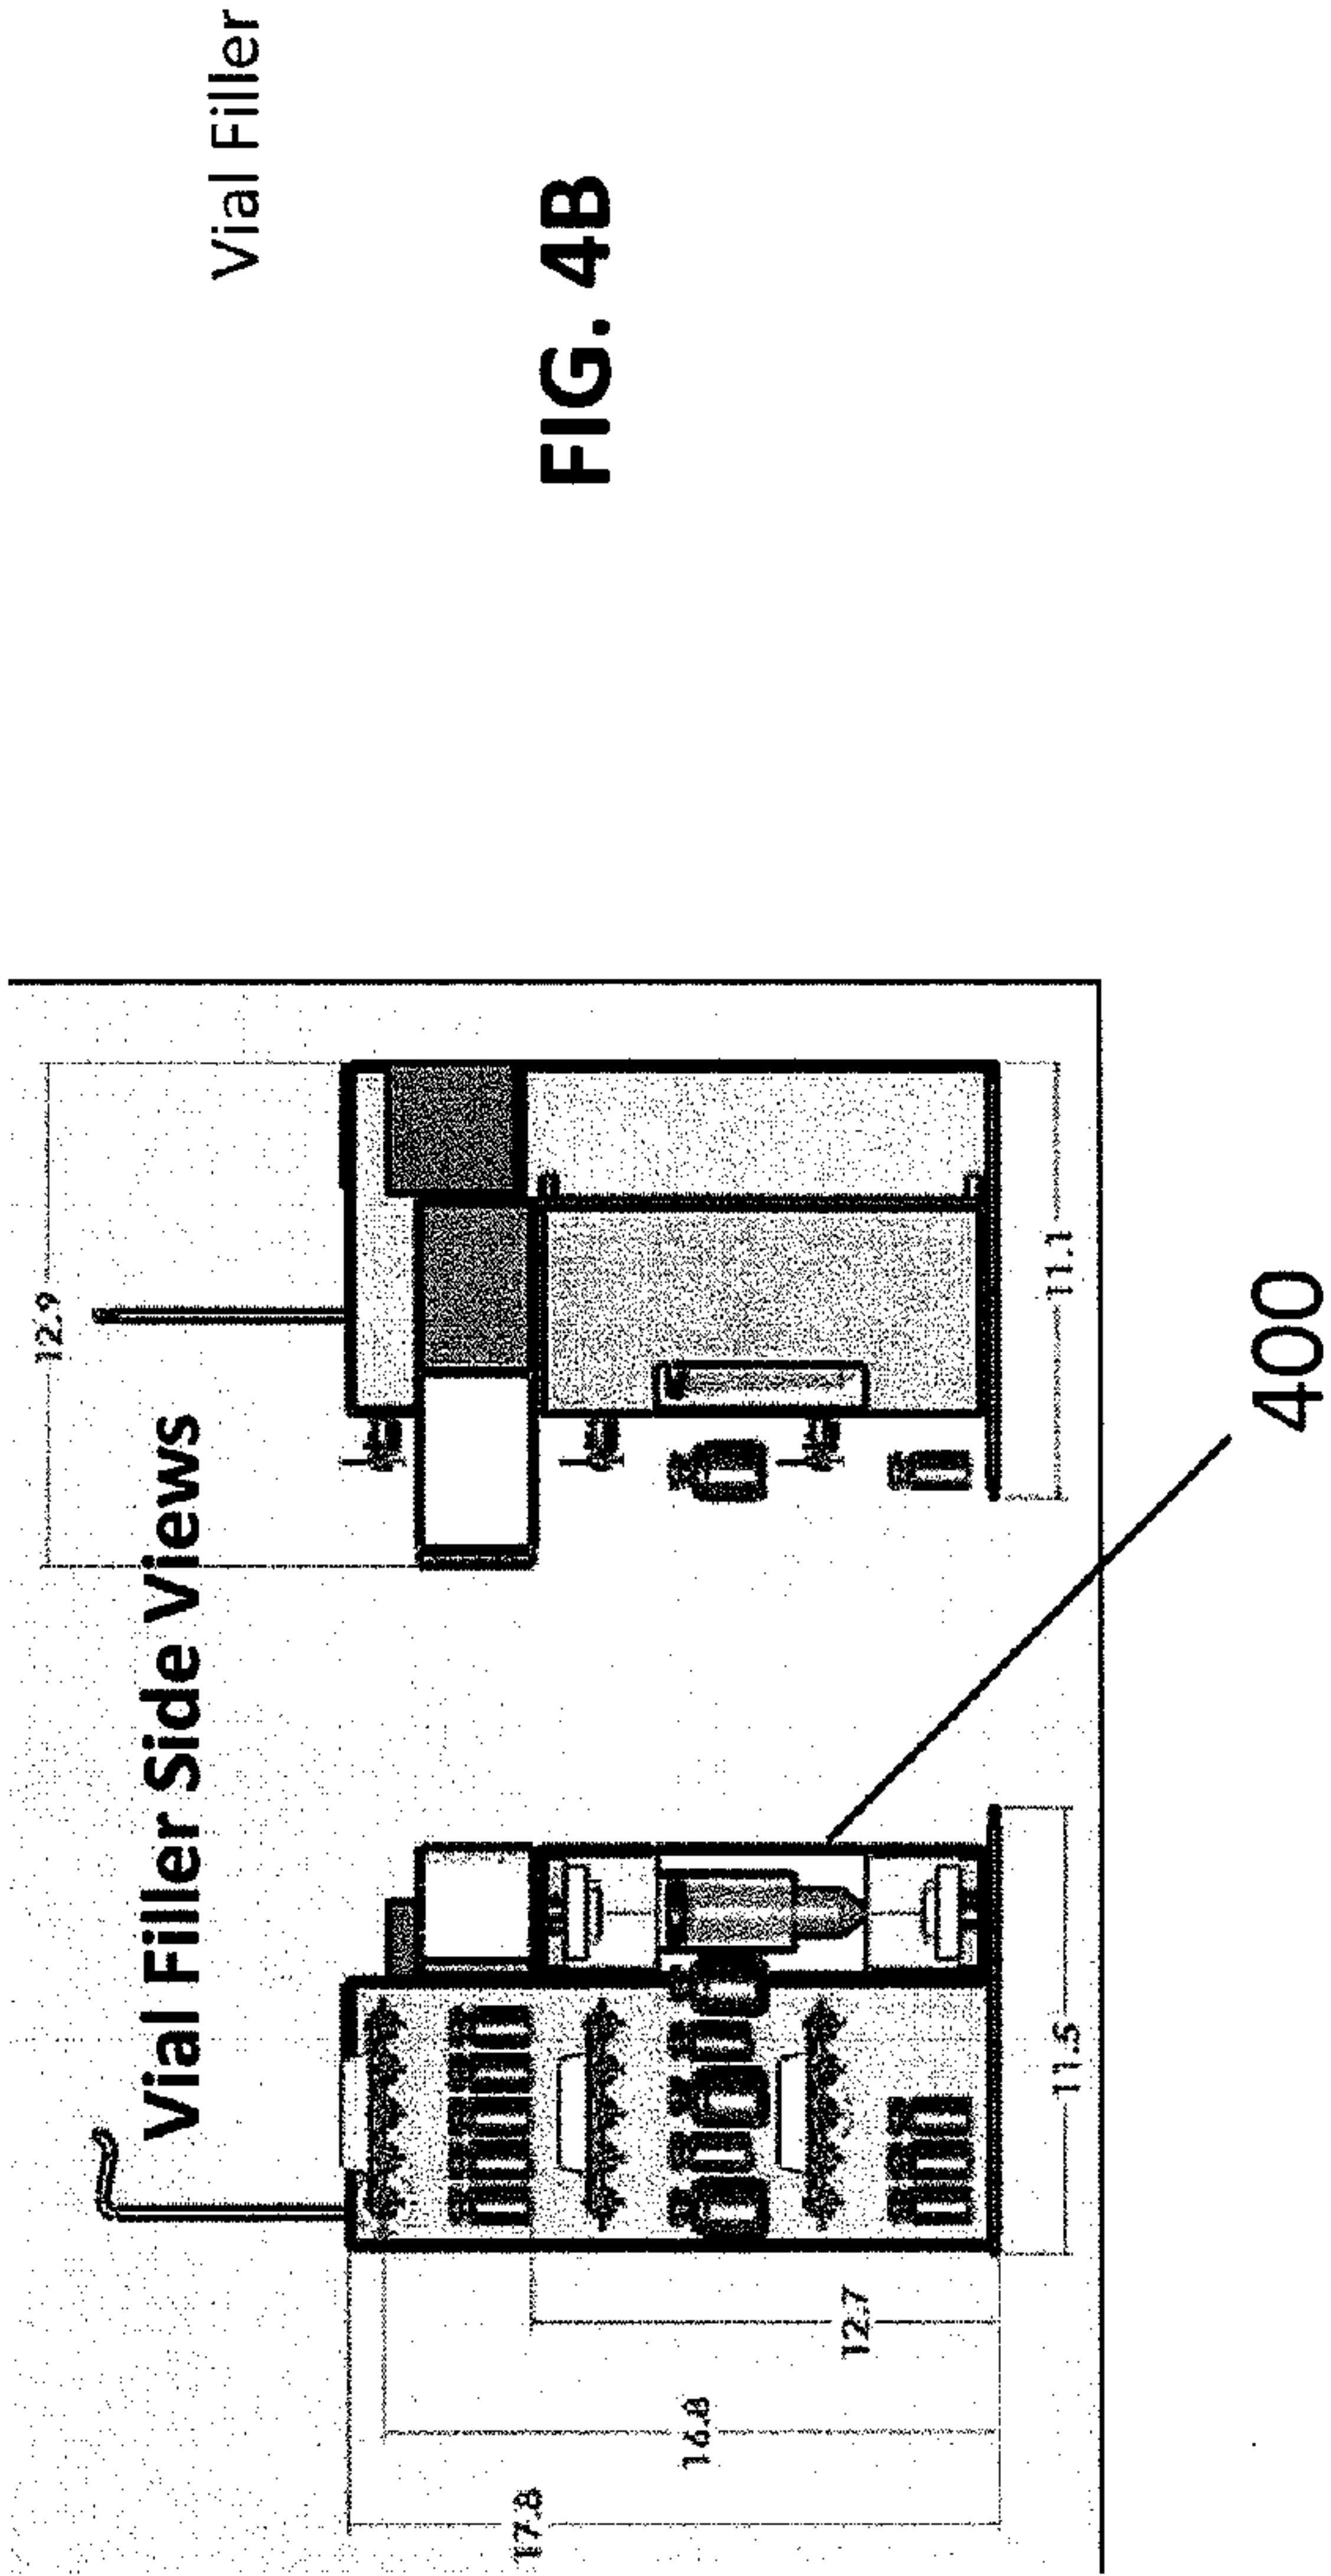

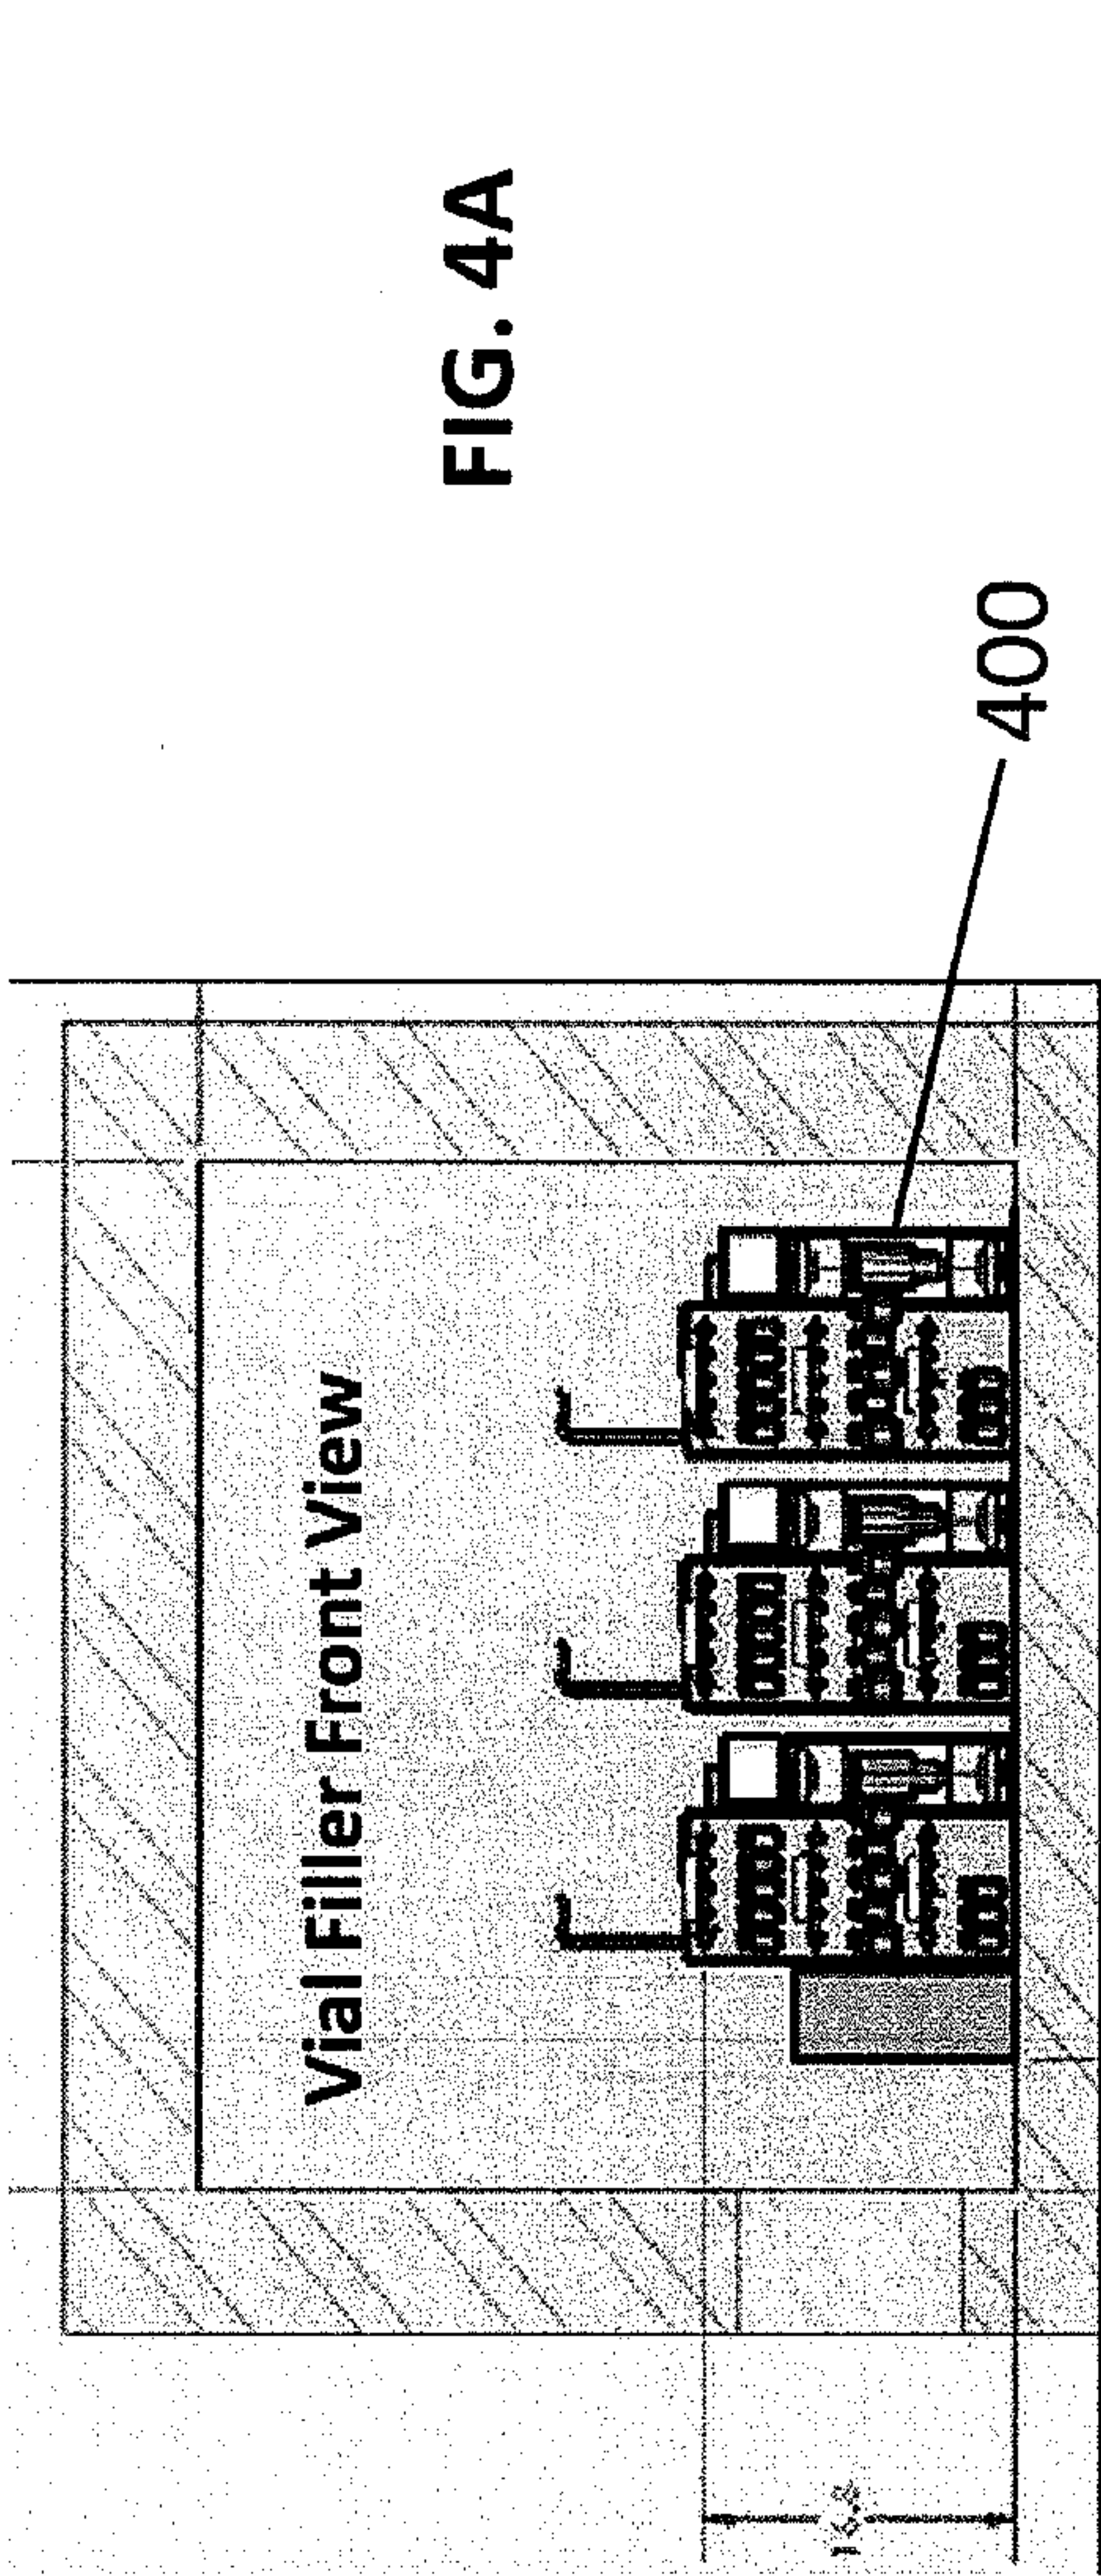



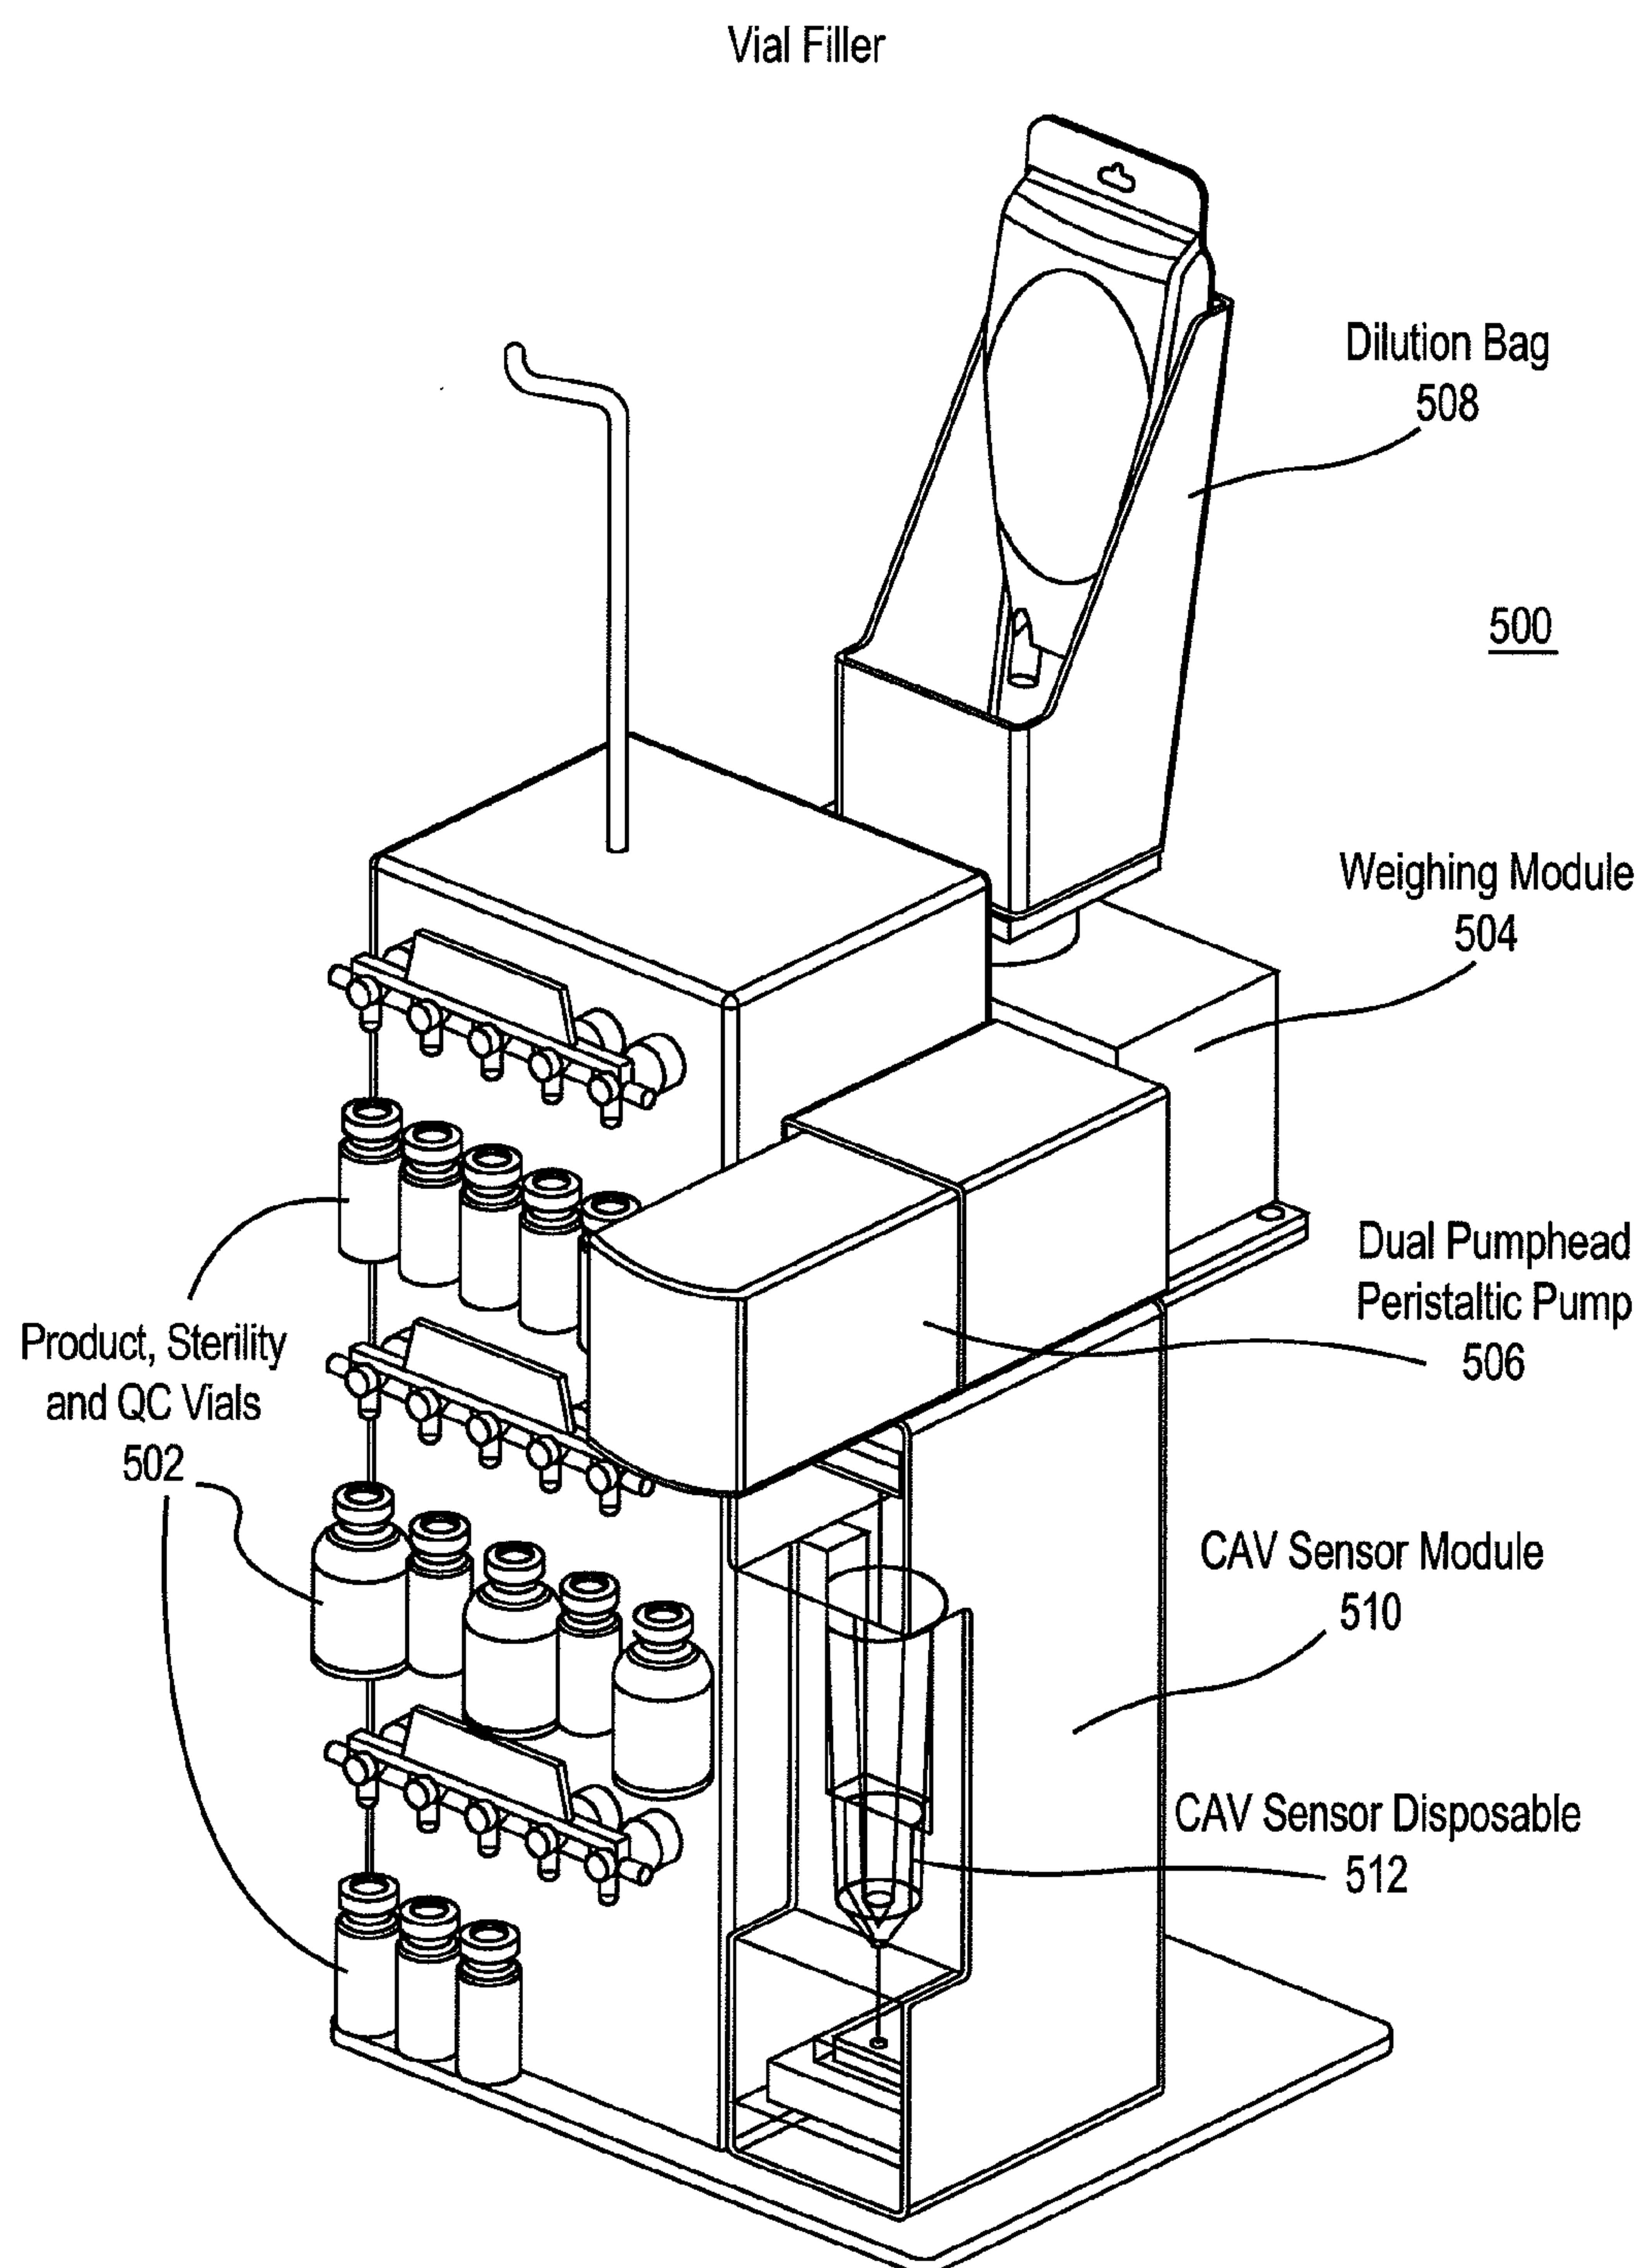


FIG. 5



Quality Control Platform


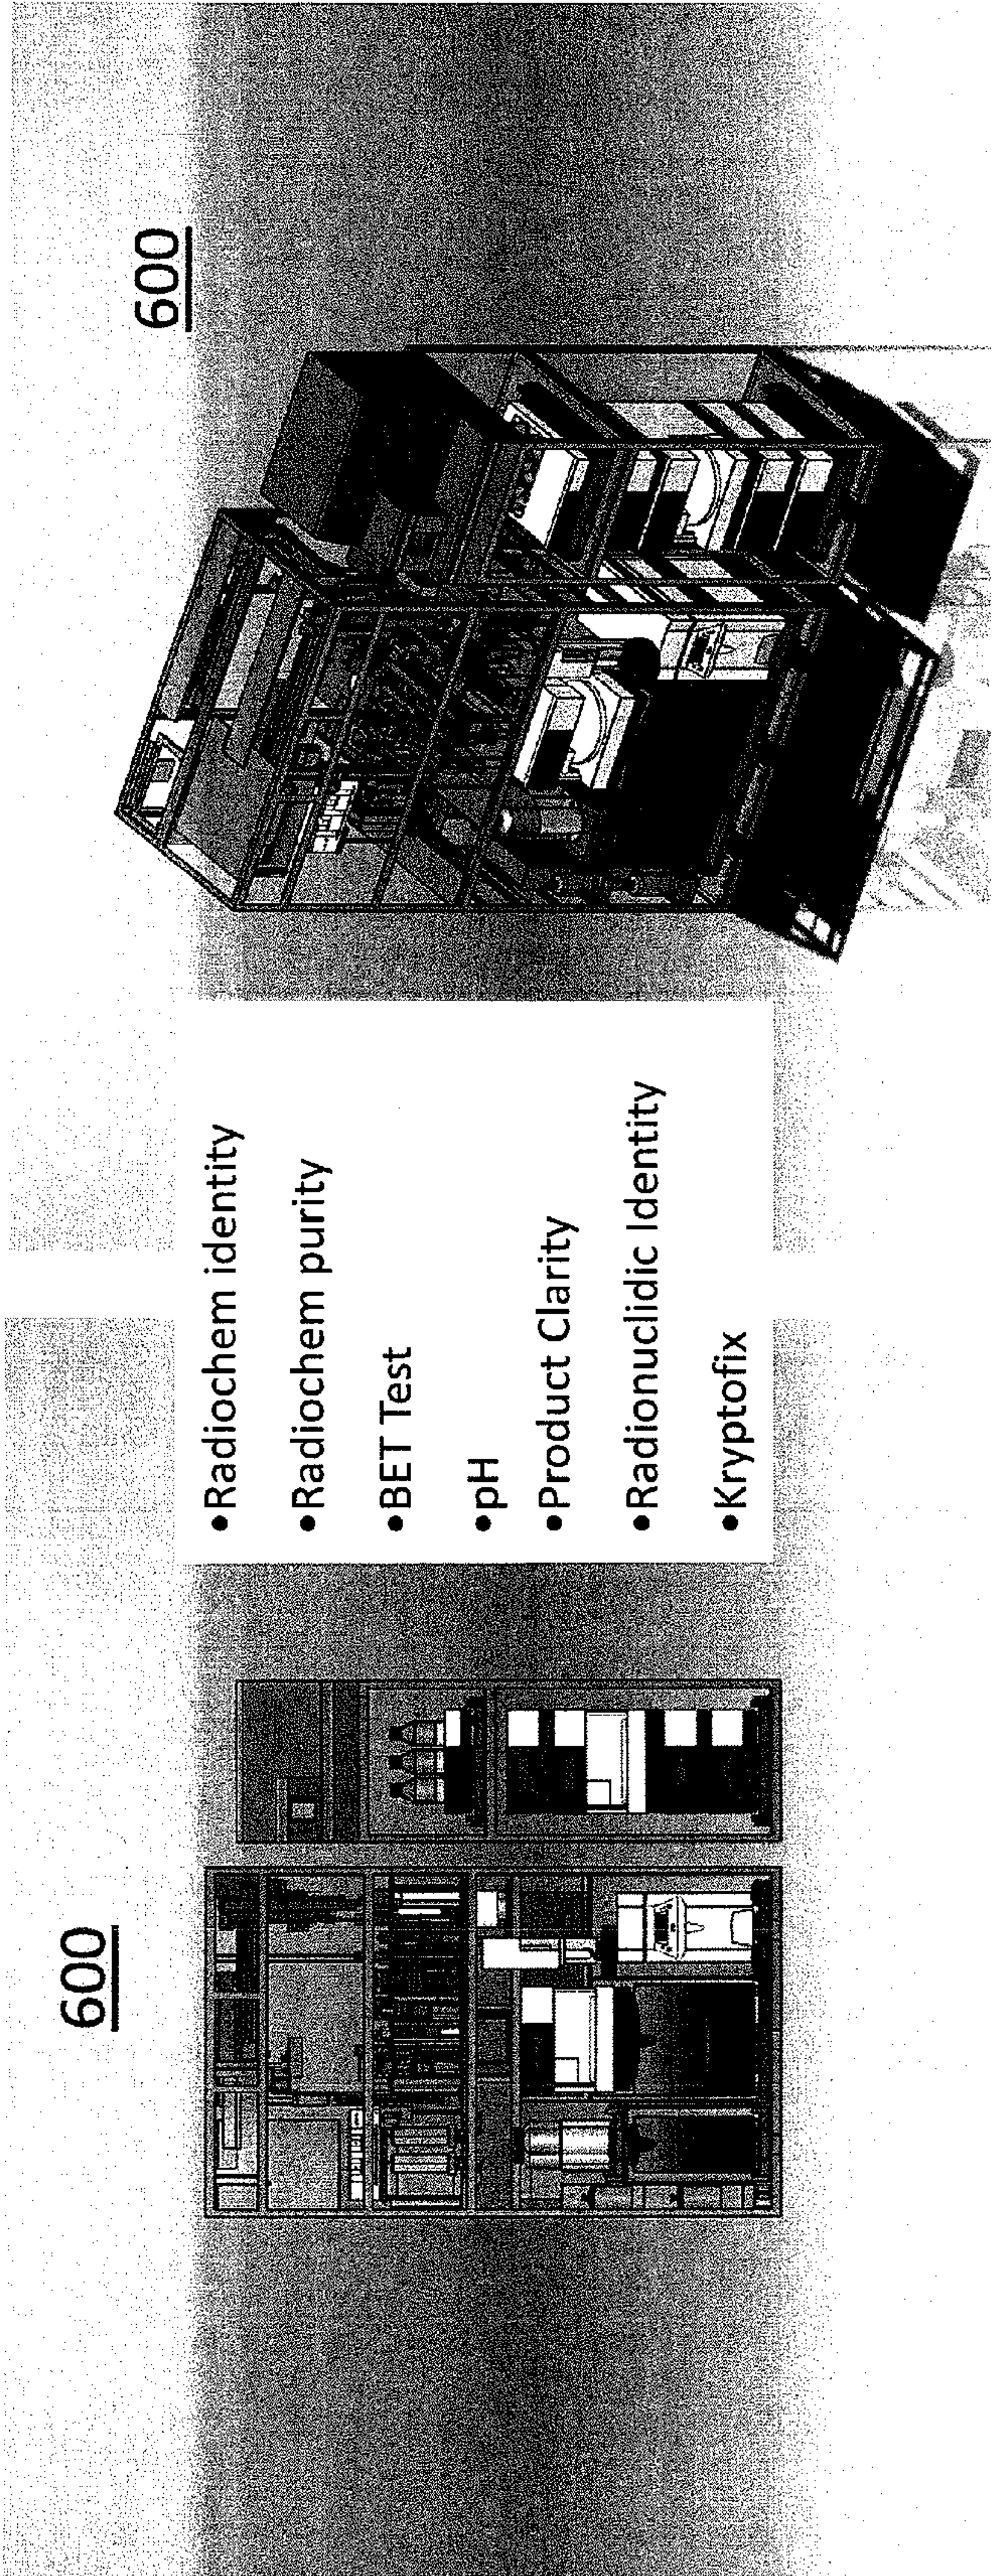



FIG. 6A

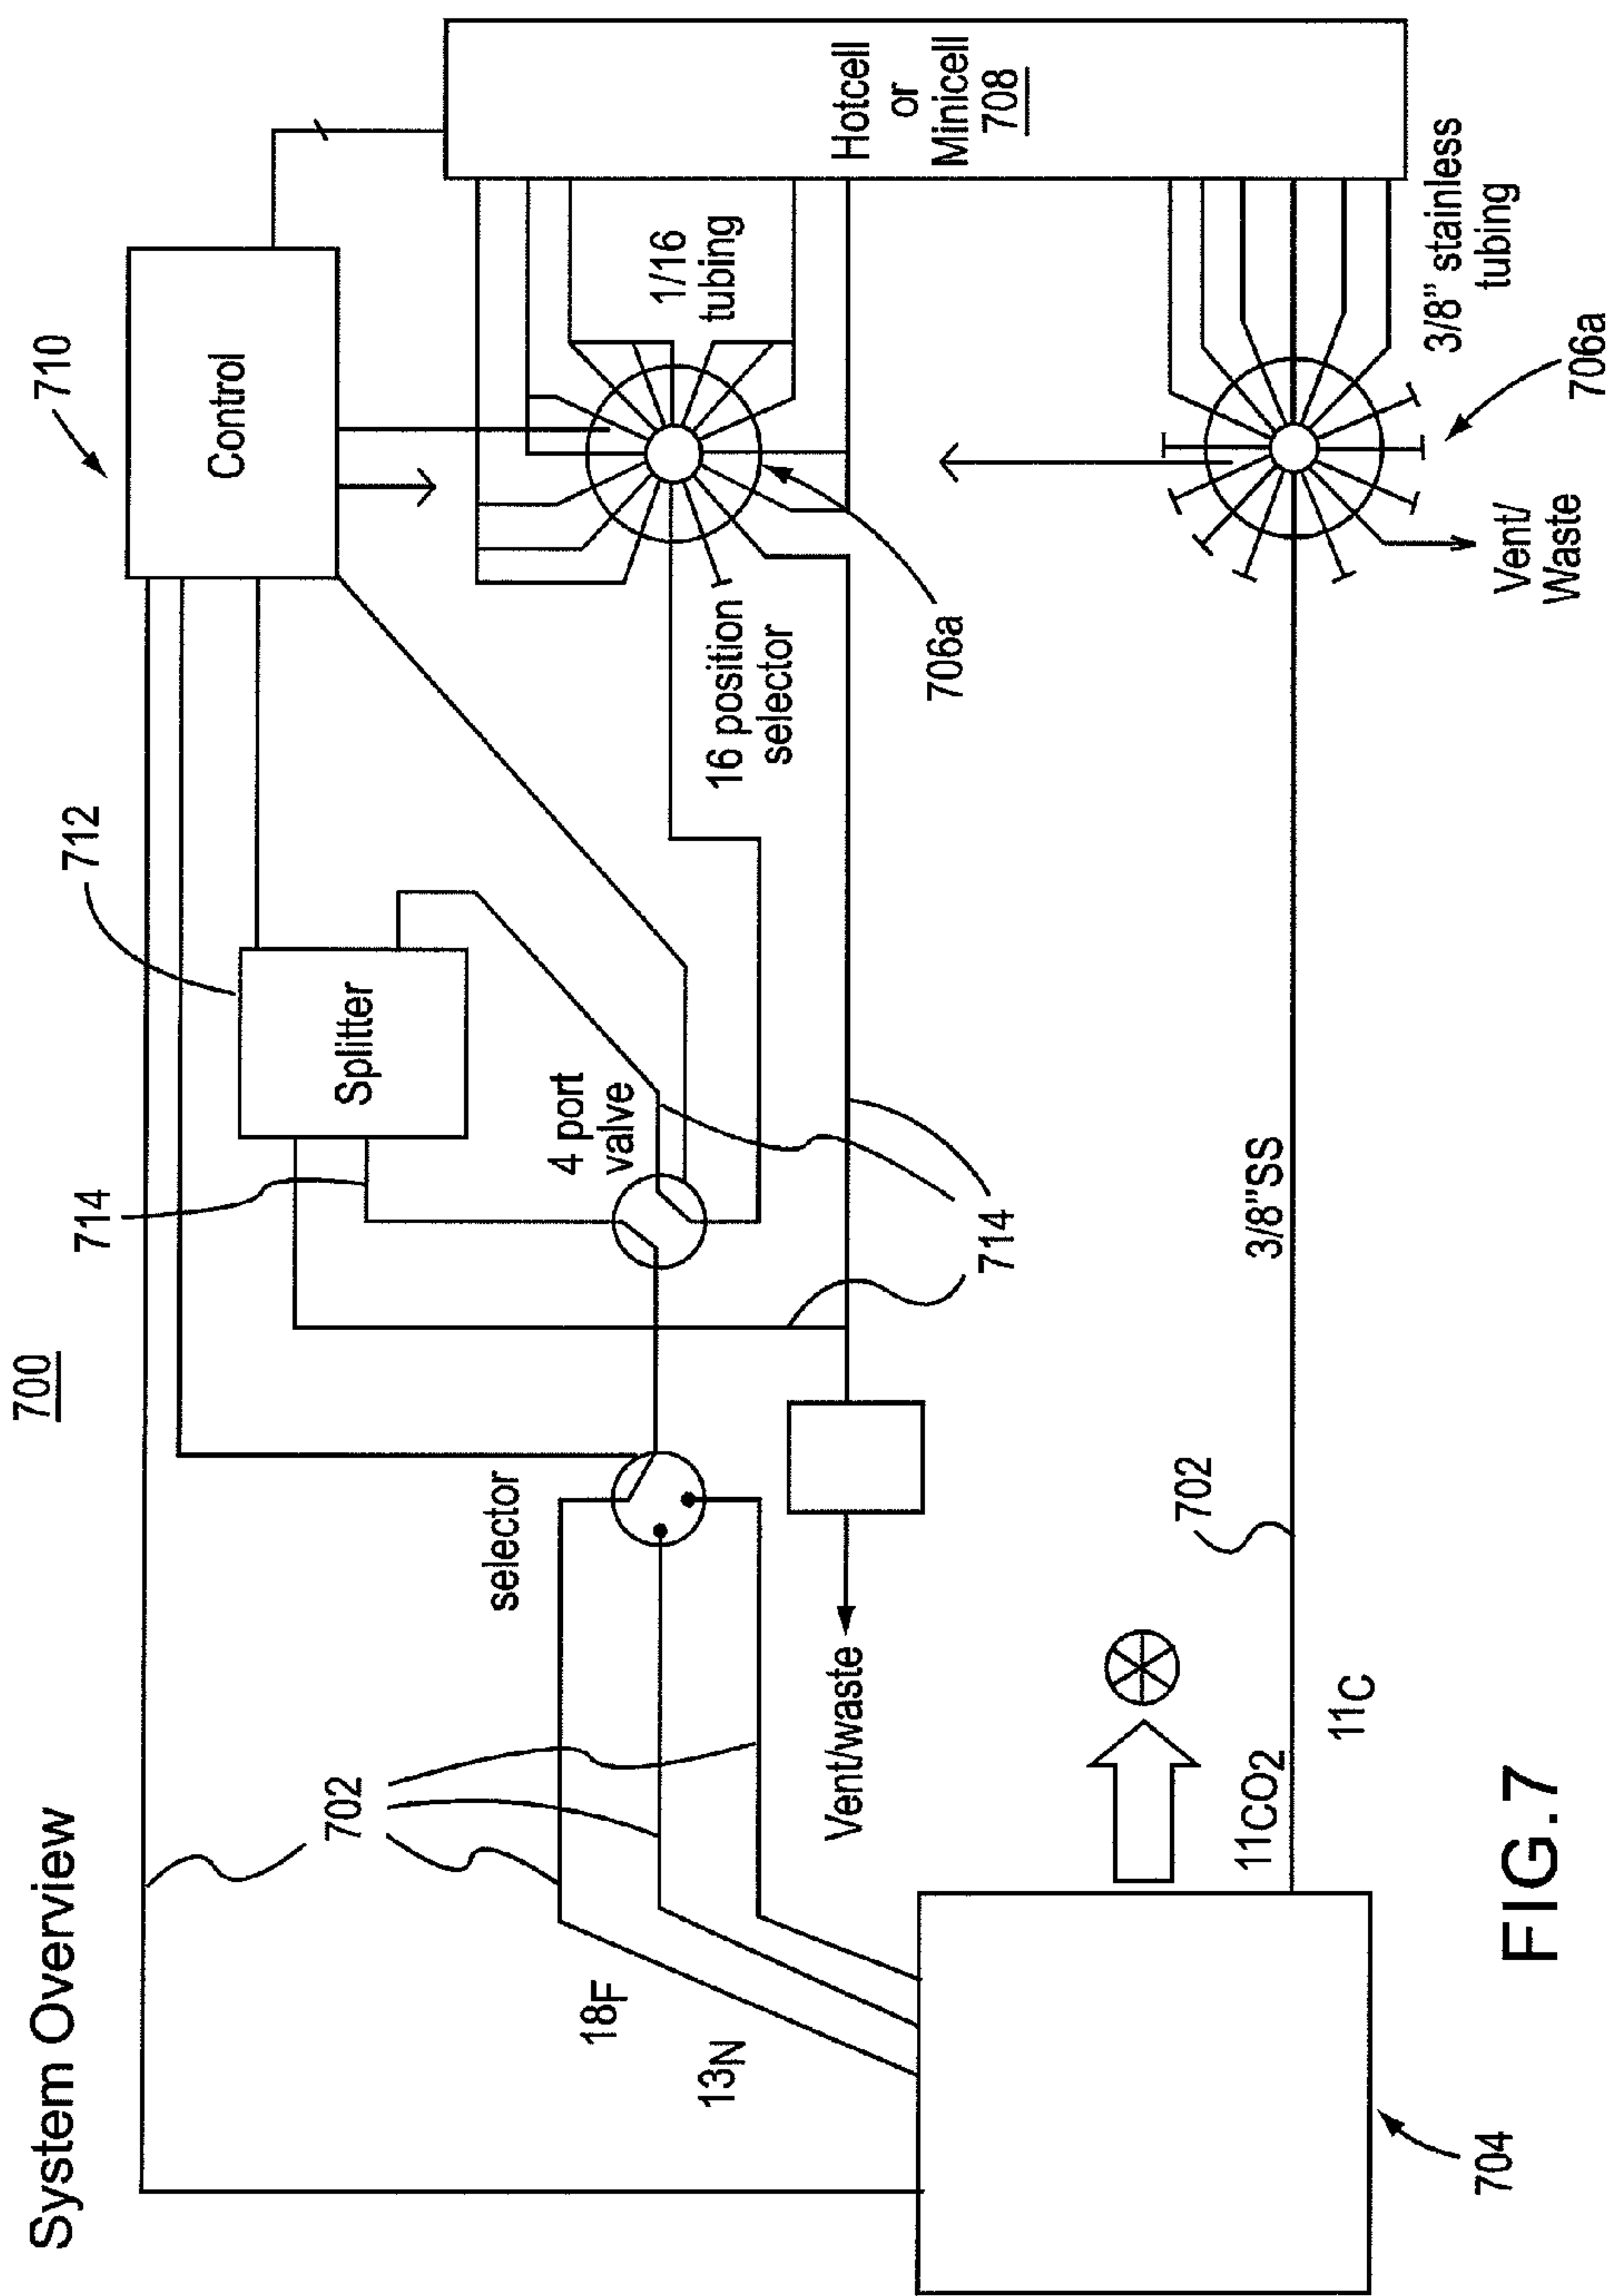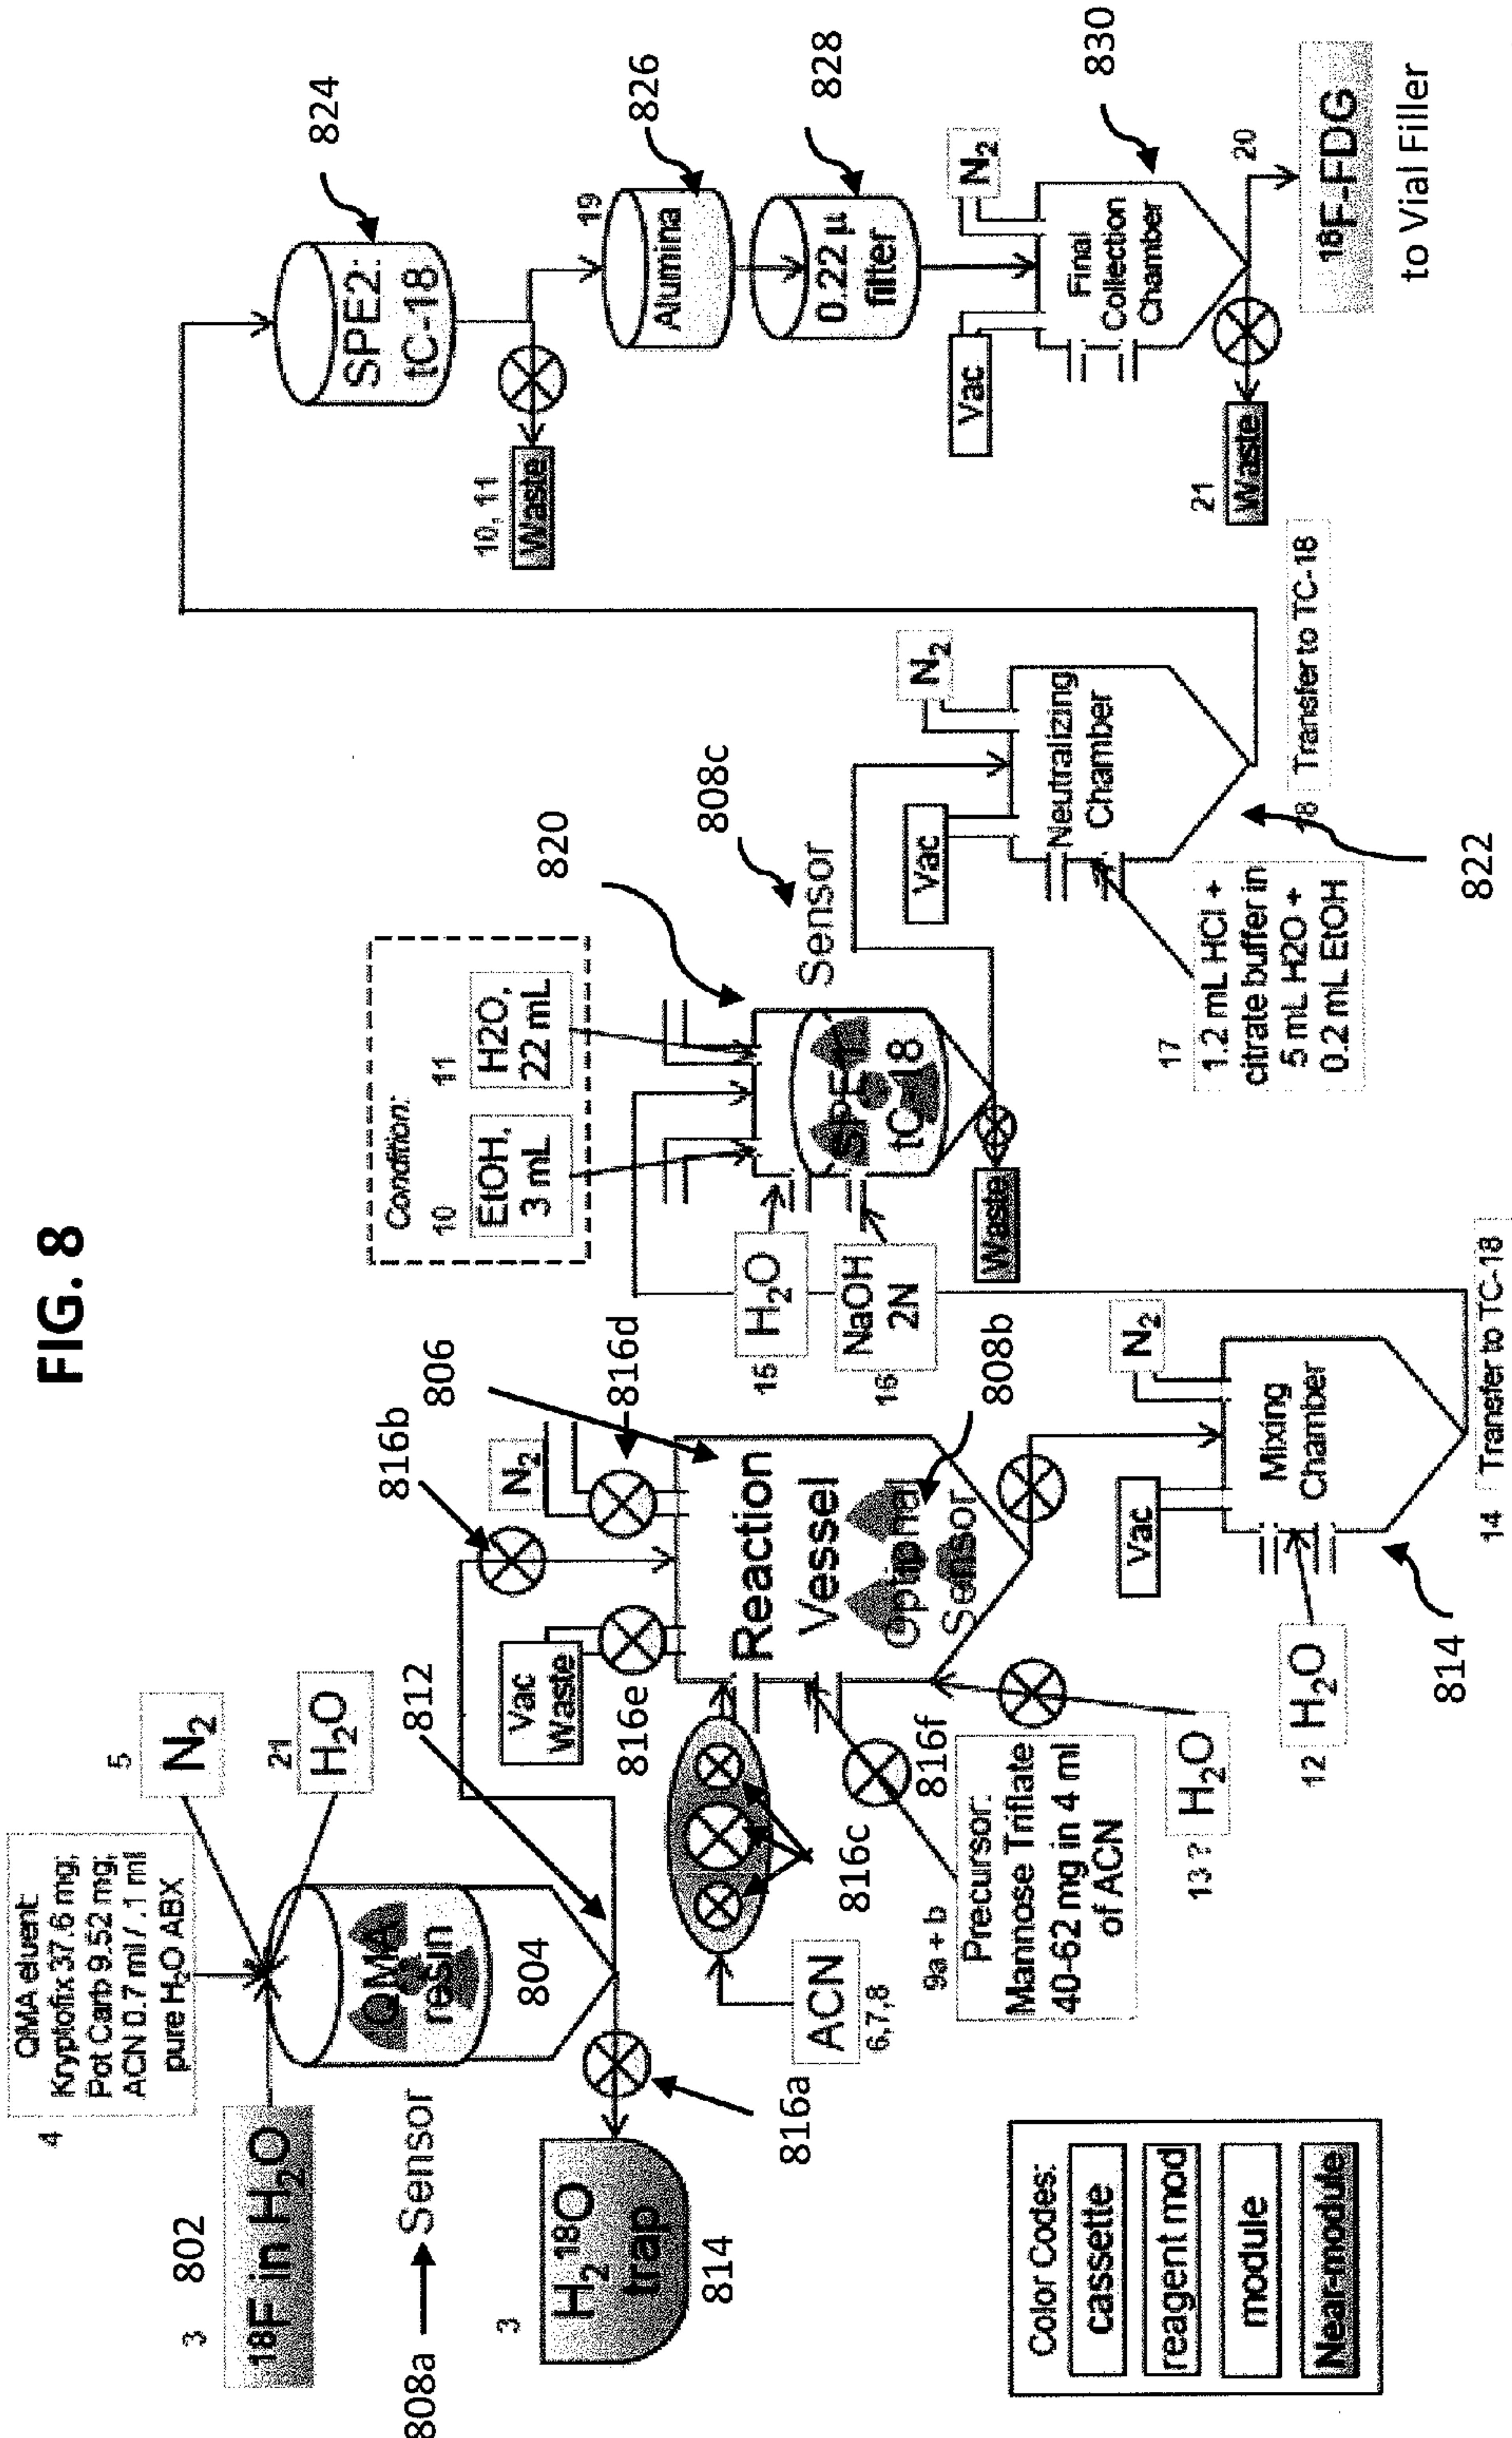FIG. 6B












process map	purpose	fluid	volume	current volume (ul)	scaled volume (ul)	reagent type	dry? cold?	entry point	module source
step ID	purpose	fluid	volume	current volume (ul)	scaled volume (ul)	reagent type	dry? cold?	entry point	module source
Process starts here if QMA doesn't need conditioning:									
3	product	F-18 in H2O	3 mL	3,000	3,000	n/a		QMA column	splitter
4	elution	K222, K2CO3, in ACN/H2O	0.8 mL	800	200	QMA Eluent	N	QMA column	n/a
5	evaporation	Nitrogen (high & low pressure)	n/a			n/a		Reaction Vessel	N2
6,7,8	drying	ACN	2.4 ml	2,400	600	ACN		Reaction Vessel	n/a
9a	labeling	ACN	4.0 ml	4,000	1,000	Precursor		Reaction Vessel	n/a
9b	labeling	Mannose Triflate (ACN from 9a dissolves)					Y		
10	SPE conditioning (2 columns)	EtOH	3 mL	3,000	750	n/a		SPE column 1 : exit below SPE column 2	n/a
11	SPE conditioning (2 columns)	H2O	22 mL	22,000	5,500	n/a		SPE column 1 : exit below SPE column 3	H2O
12	sample dilution	H2O	22 mL	22,000	5,500	n/a		Reaction Vessel, or after	H2O
13	rinse RV walls	H2O	4 mL	4,000	1,000	n/a		Reaction Vessel	H2O
14	Transfer fluid onto TC18 column	sum of steps 4,6,7,8,9,12,13:		33,200	8,300				
15	washing	H2O	46 mL	46,000	11,500	n/a		TC18 column	H2O
16	hydrolysis / elution	NaOH, 2N	0.75 mL	750	188	NaOH		TC18 column	n/a
17	neutralize pH	citrate buffer + HCl + EtOH + H2O	6.4 mL	6,400	1,600	neutralizing reagent	N	neutralizing chamber	n/a
18	Transfer fluid onto TC18 column	sum of steps 16,17:		7,150	1,788				
19	Push fluid through Alumina cartridge and 0.22 micron filter	n/a	n/a	n/a	n/a	n/a		n/a	
20	Transfer fluid to hot cell	depends on whether TC18 is eluted	TBD						
21	flush cassette	H2O	TBD					TBD: possibly several	H2O
volume totals									
	Flows into Neutralizing Chamber		uL	1,788					
	Flows through to waste		uL	21,970					
	stored in reagent pack		uL	17,350	4,338				
	pumped from module		uL	94,000	23,500				
	combined		uL	111,350	27,838				

FIG. 9



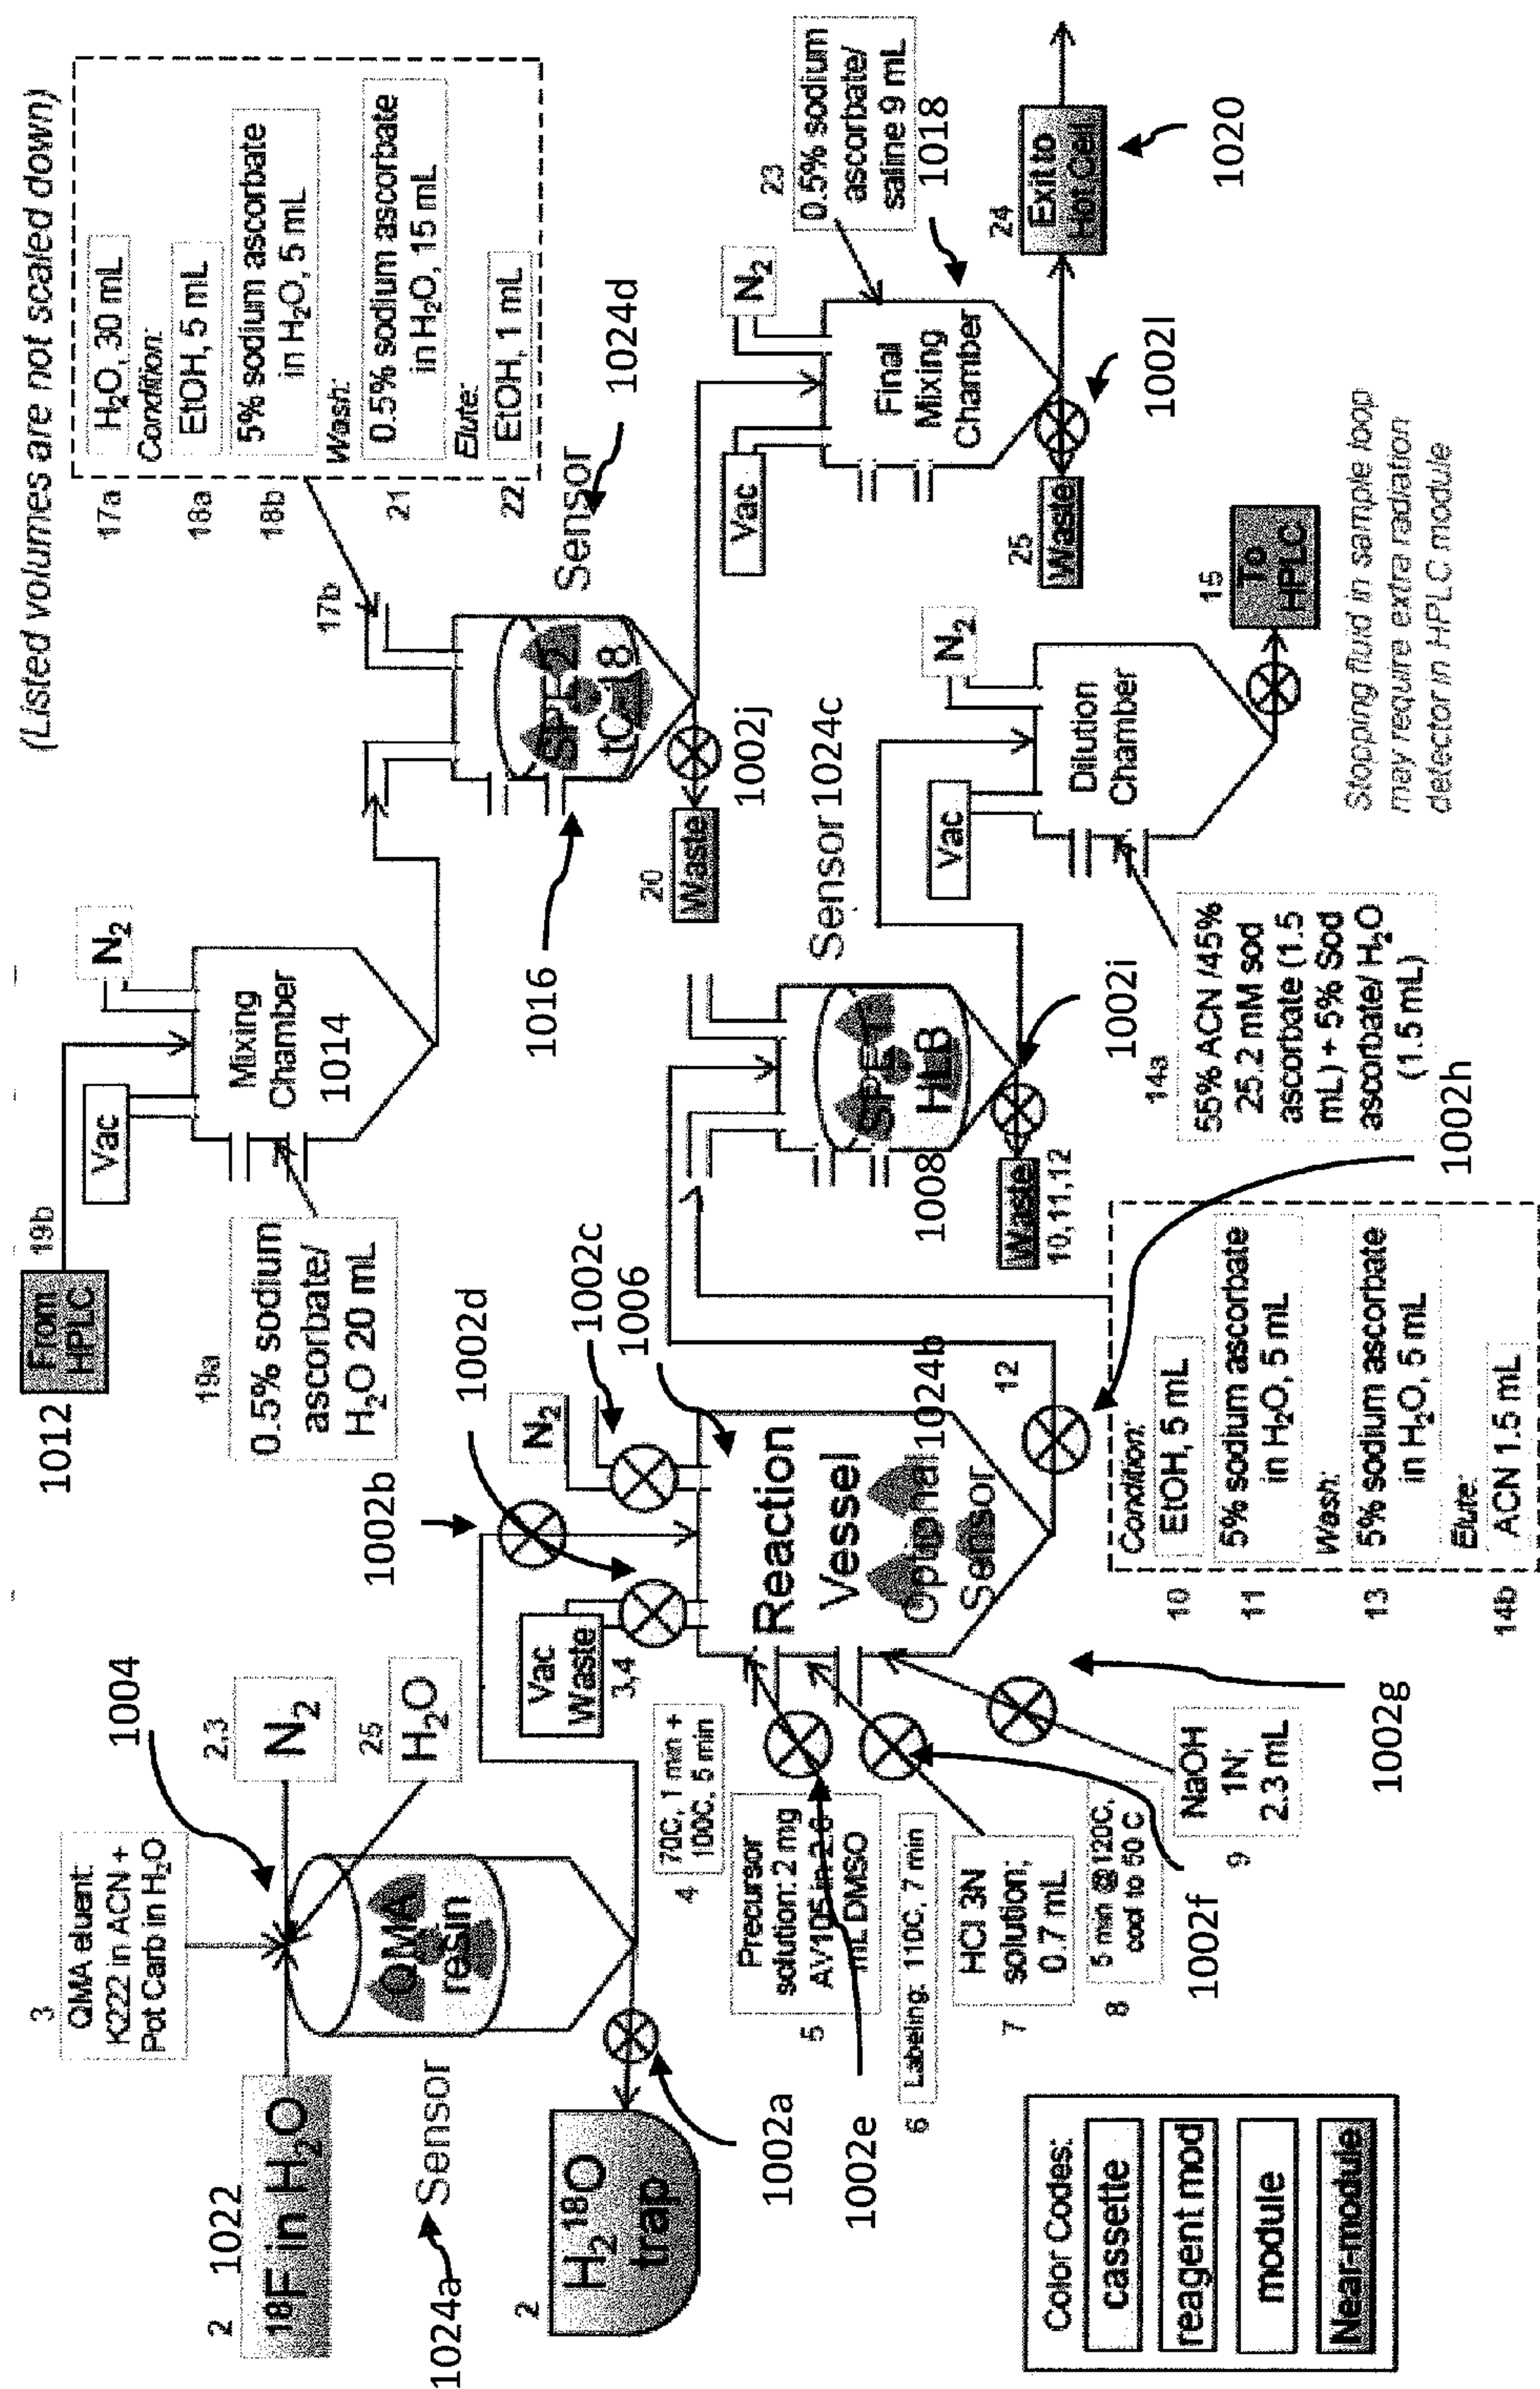


**FIG. 10**



process map	purpose	fluid	volume	current volume (uL)	scaled volume (uL)	reagent name	dry? cold?	entry point	module source
2	product	P-18 in H2O-18	3 mL	3,000	3,000	splitter bolus	N	QMA column	n/a
3	elution	K222, K2CD3 in ACN/H2O	0.6 ml	600	150	QMA Eluent	N	QMA column	n/a
	raise temp in RV; to 70C for 1 min, then to 200C for 5 min, then to 210C (see step 6)	n/a	n/a	n/a	n/a	n/a		n/a	n/a
4		2.0 mg AVUS	n/a	n/a	n/a	Precursor	Y	mixed in Reagent Pack	n/a
5a	powder for mixing precursor	DMSO	2 - 2.6 mL	2,300	575	Precursor		Reaction Vessel	n/a
5b	solvent for mixing precursor	n/a	n/a	n/a	n/a	n/a		n/a	n/a
6	Labeling: 7 min @ 10C	HCl 3N	0.7 mL	700	175	Hydralyzer		Reaction Vessel	n/a
7	hydrolysis	n/a	n/a	n/a	n/a	n/a		n/a	n/a
8	5 min @ 120C	Coolant fluid (H2O or N2)	750	n/a	n/a	n/a		n/a	n/a
9	neutralization	NaOH, 1N	2.3 mL	2,300	575	Neutralizer		Reaction Vessel	n/a
10	HLB conditioning	EtOH	5 mL	5,000	1,250	HLB conditioner1		HLB column	n/a
11	HLB conditioning	5% sodium ascorbate / H2O	5 mL	5,000	1,250	HLB conditioner2	Y	HLB column	n/a
12	Transfer fluid onto C18 column	sum of steps 5, 6, 7, 9, 10, 11		5,900	1,475				
13	HLB washing	5% sodium ascorbate / H2O	5 mL	5,000	1,250	HLB wash	Y	HLB column	n/a
14a	Dilution formulation for HPLC	55% ACN/45% 25.2 mM sod ascorbate + 5% sod ascorbate/H2O	3.0 mL	3,000	750	mobile phase match	Y	dilution vial	n/a
14b	HLB elution	ACN	1.5 ml	1,500	375	HLB eluant		HLB column	n/a
15	Transfer fluid to HPLC	sum of steps 14a, 14b	n/a	4,500	1,125	n/a		HPLC	n/a
16	Inject sample and acquire data	n/a	n/a	n/a	n/a	n/a		HPLC	n/a
17a	solvent rinse	H2O	30 ml	30,000	7,500	solvent rinse		C18 column	n/a
17b	remove water	N2	n/a	n/a	n/a	blow dry		C18 column	n/a
18a	C18 conditioning	EtOH	5 mL	5,000	1,250	tc18 conditioner1		C18 column	n/a
18b	C18 conditioning	5% sodium ascorbate / H2O	5 mL	5,000	1,250	tc18 conditioner2	Y	C18 column	n/a
19a	Dilution for C18 for binding of product	0.5% sodium ascorbate / H2O	20 mL	20,000	5,000	Pre-SPE Diluent	Y	Dilution for C18 for binding of product	n/a
19b	product	product identified in HPLC	4 - 12 mL	8,000	2,000	n/a	N	binding of product	n/a
20	Transfer fluid onto C18 column	sum of steps 19a, 19b		28,000	7,000			making vial	n/a
21	washing	0.5% sodium ascorbate / H2O	15 ml	15,000	3,750	tc18 wash	Y	C18 column	n/a
22	elution	EtOH	1 ml	1,000	250	tc18 eluant	N	C18 column	n/a
23	reformulation for dosing	0.5% sodium ascorbate in saline	9 mL	9,000	2,250	Final Diluent	Y	Final syringe	n/a
24	Transfer fluid to hot cell	sum of steps 22, 23		10,000	2,500				
25	flush cassette	H2O	750			n/a		TBD: possible several	n/a
	clear line	Nitrogen (high & low pressure)	n/a			n/a		inlet reservoir	n/a
	cooling - external	compressed air	n/a			n/a		Reaction Vessel	n/a
		stored in reagent pack	ul	75,400	18,850				
		pumped from module	ul	35,000	8,750				
		combined	ul	110,400	27,600				

FIG. 11



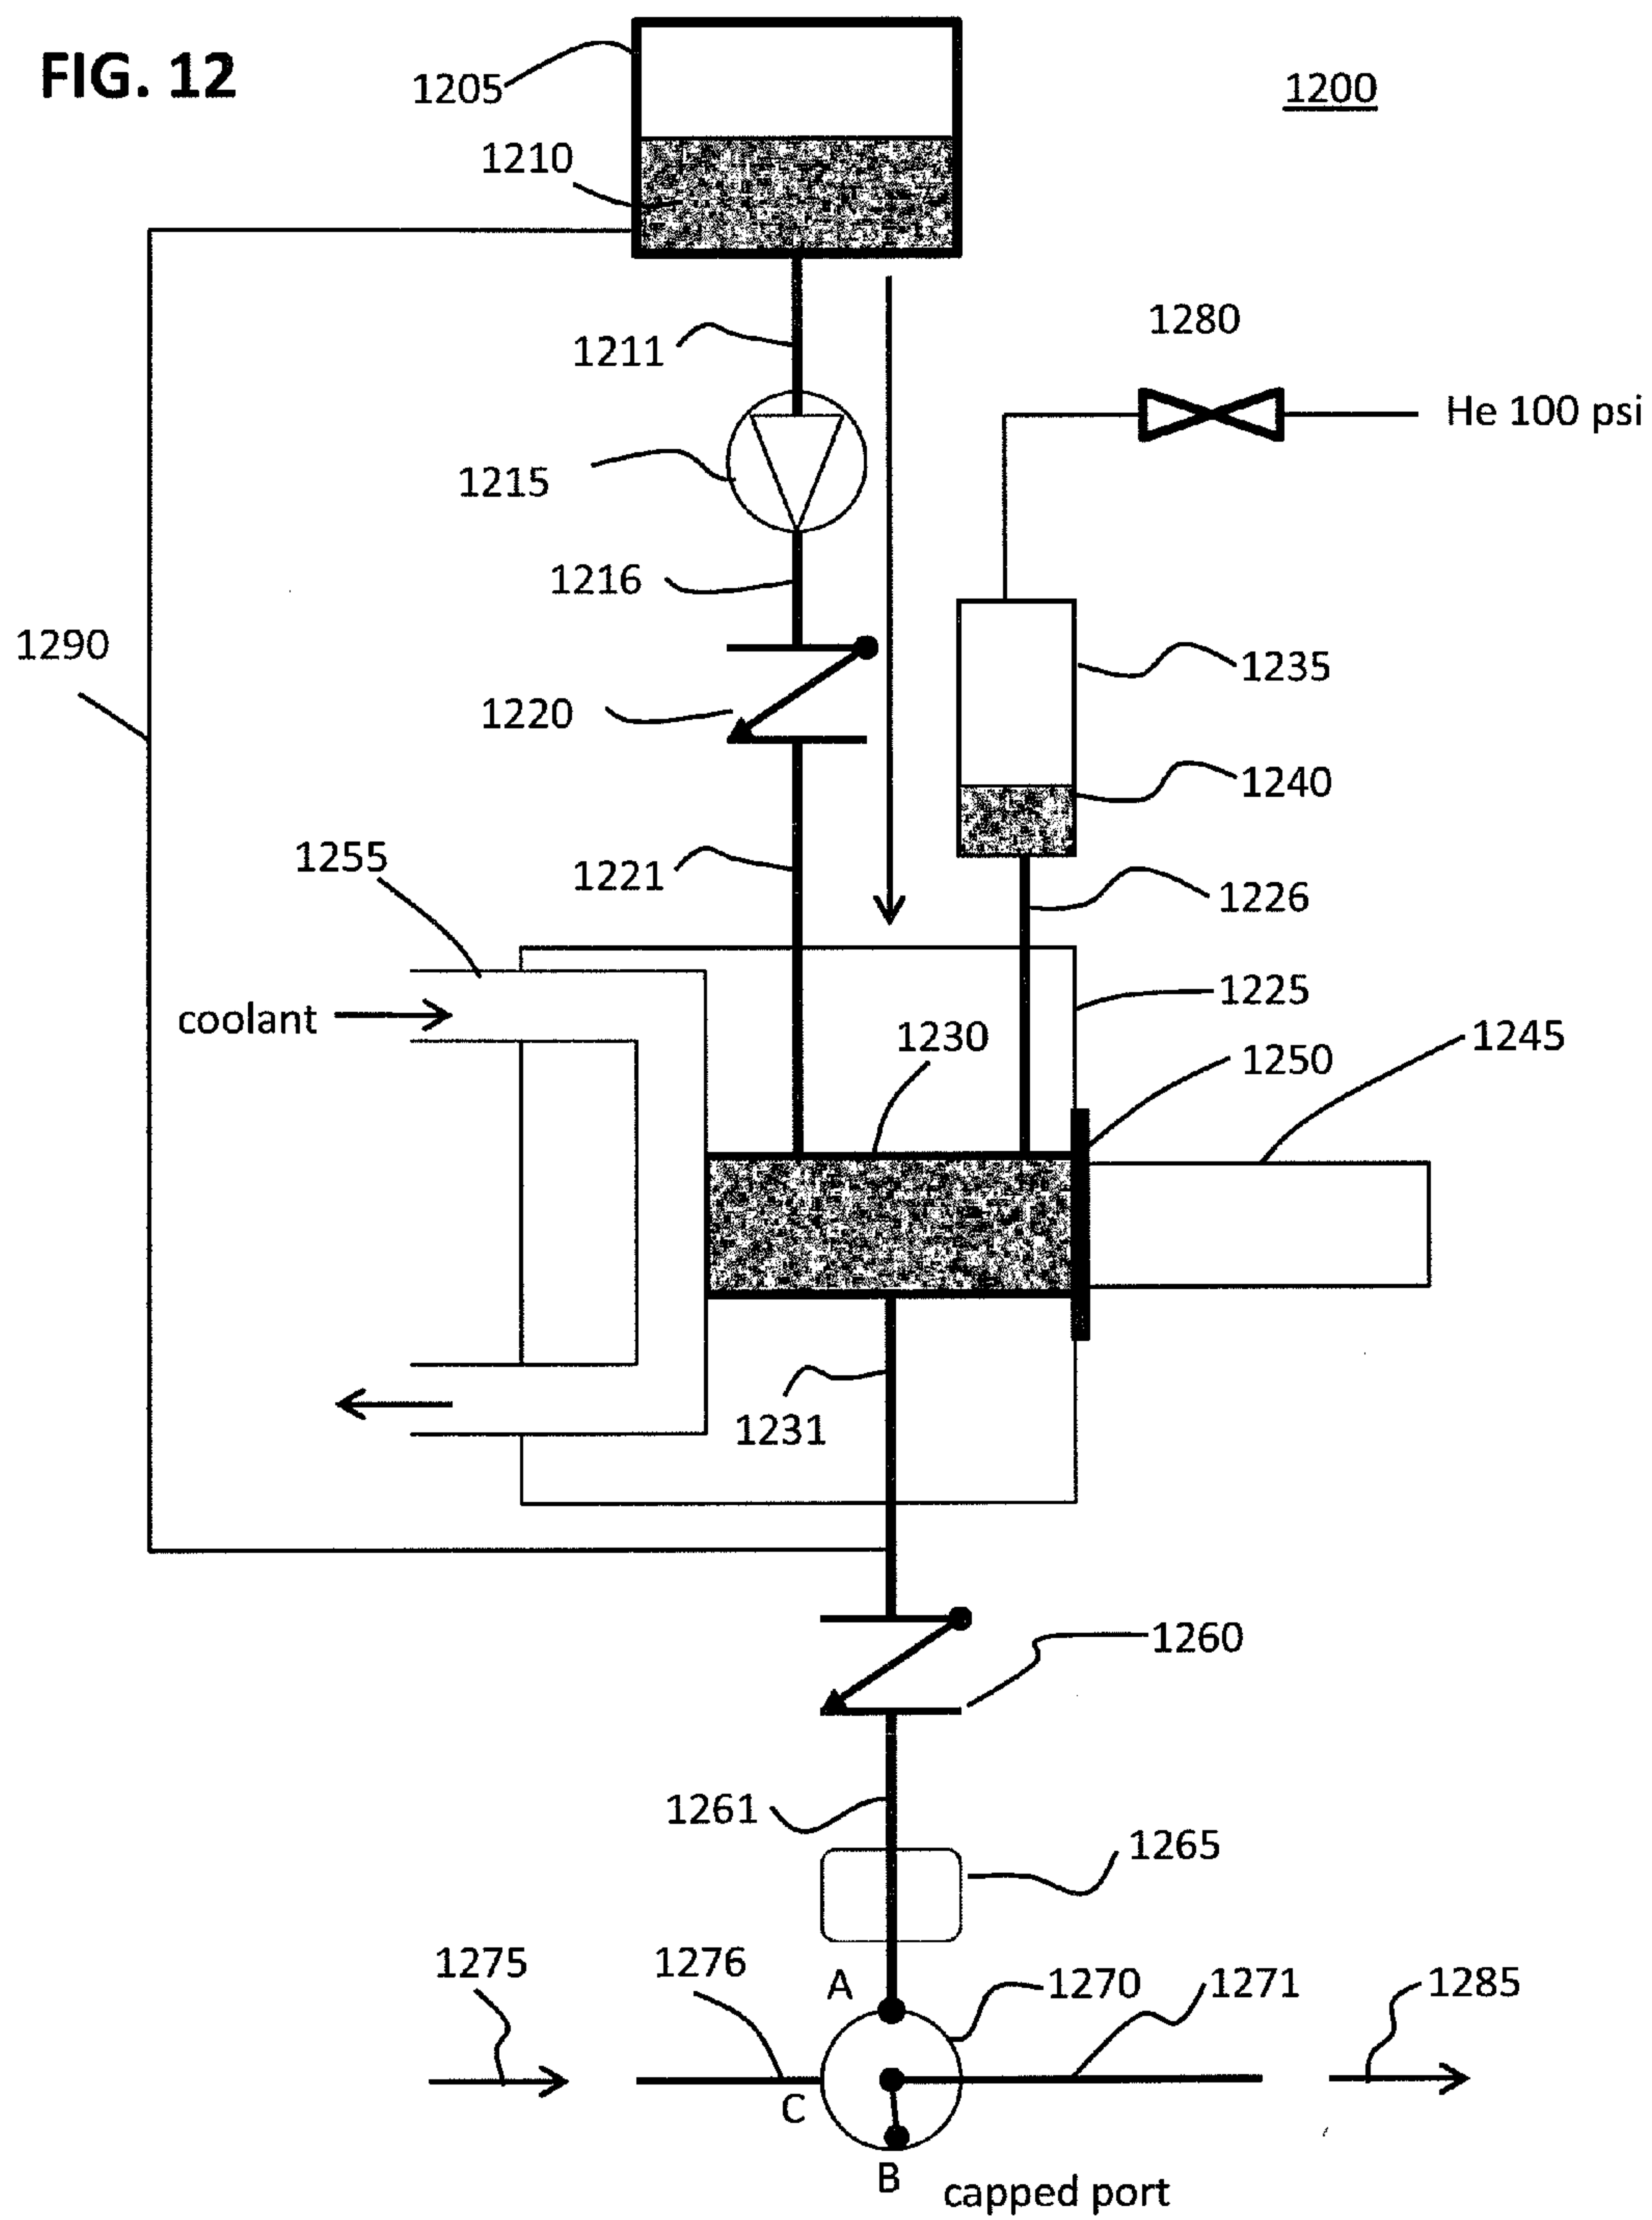



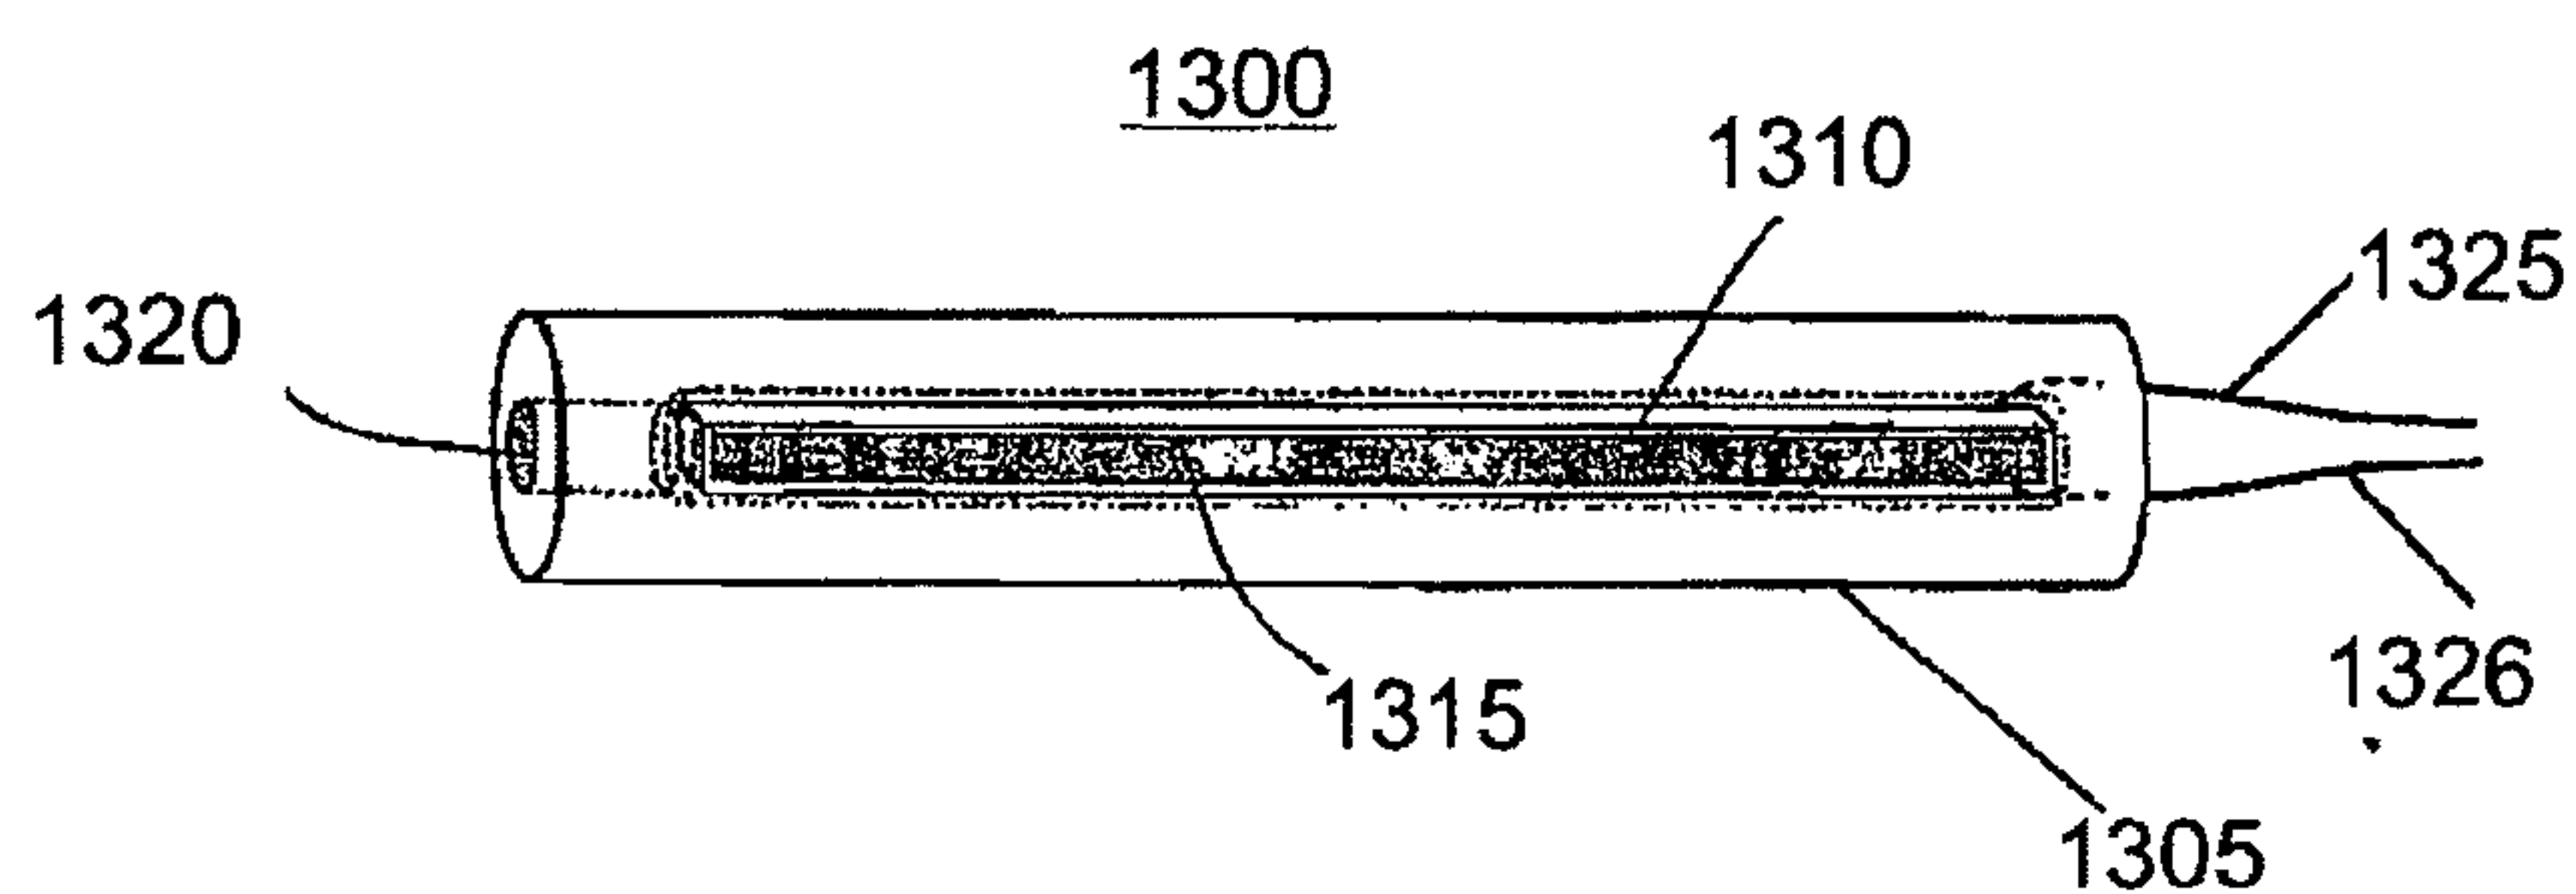


FIG. 13

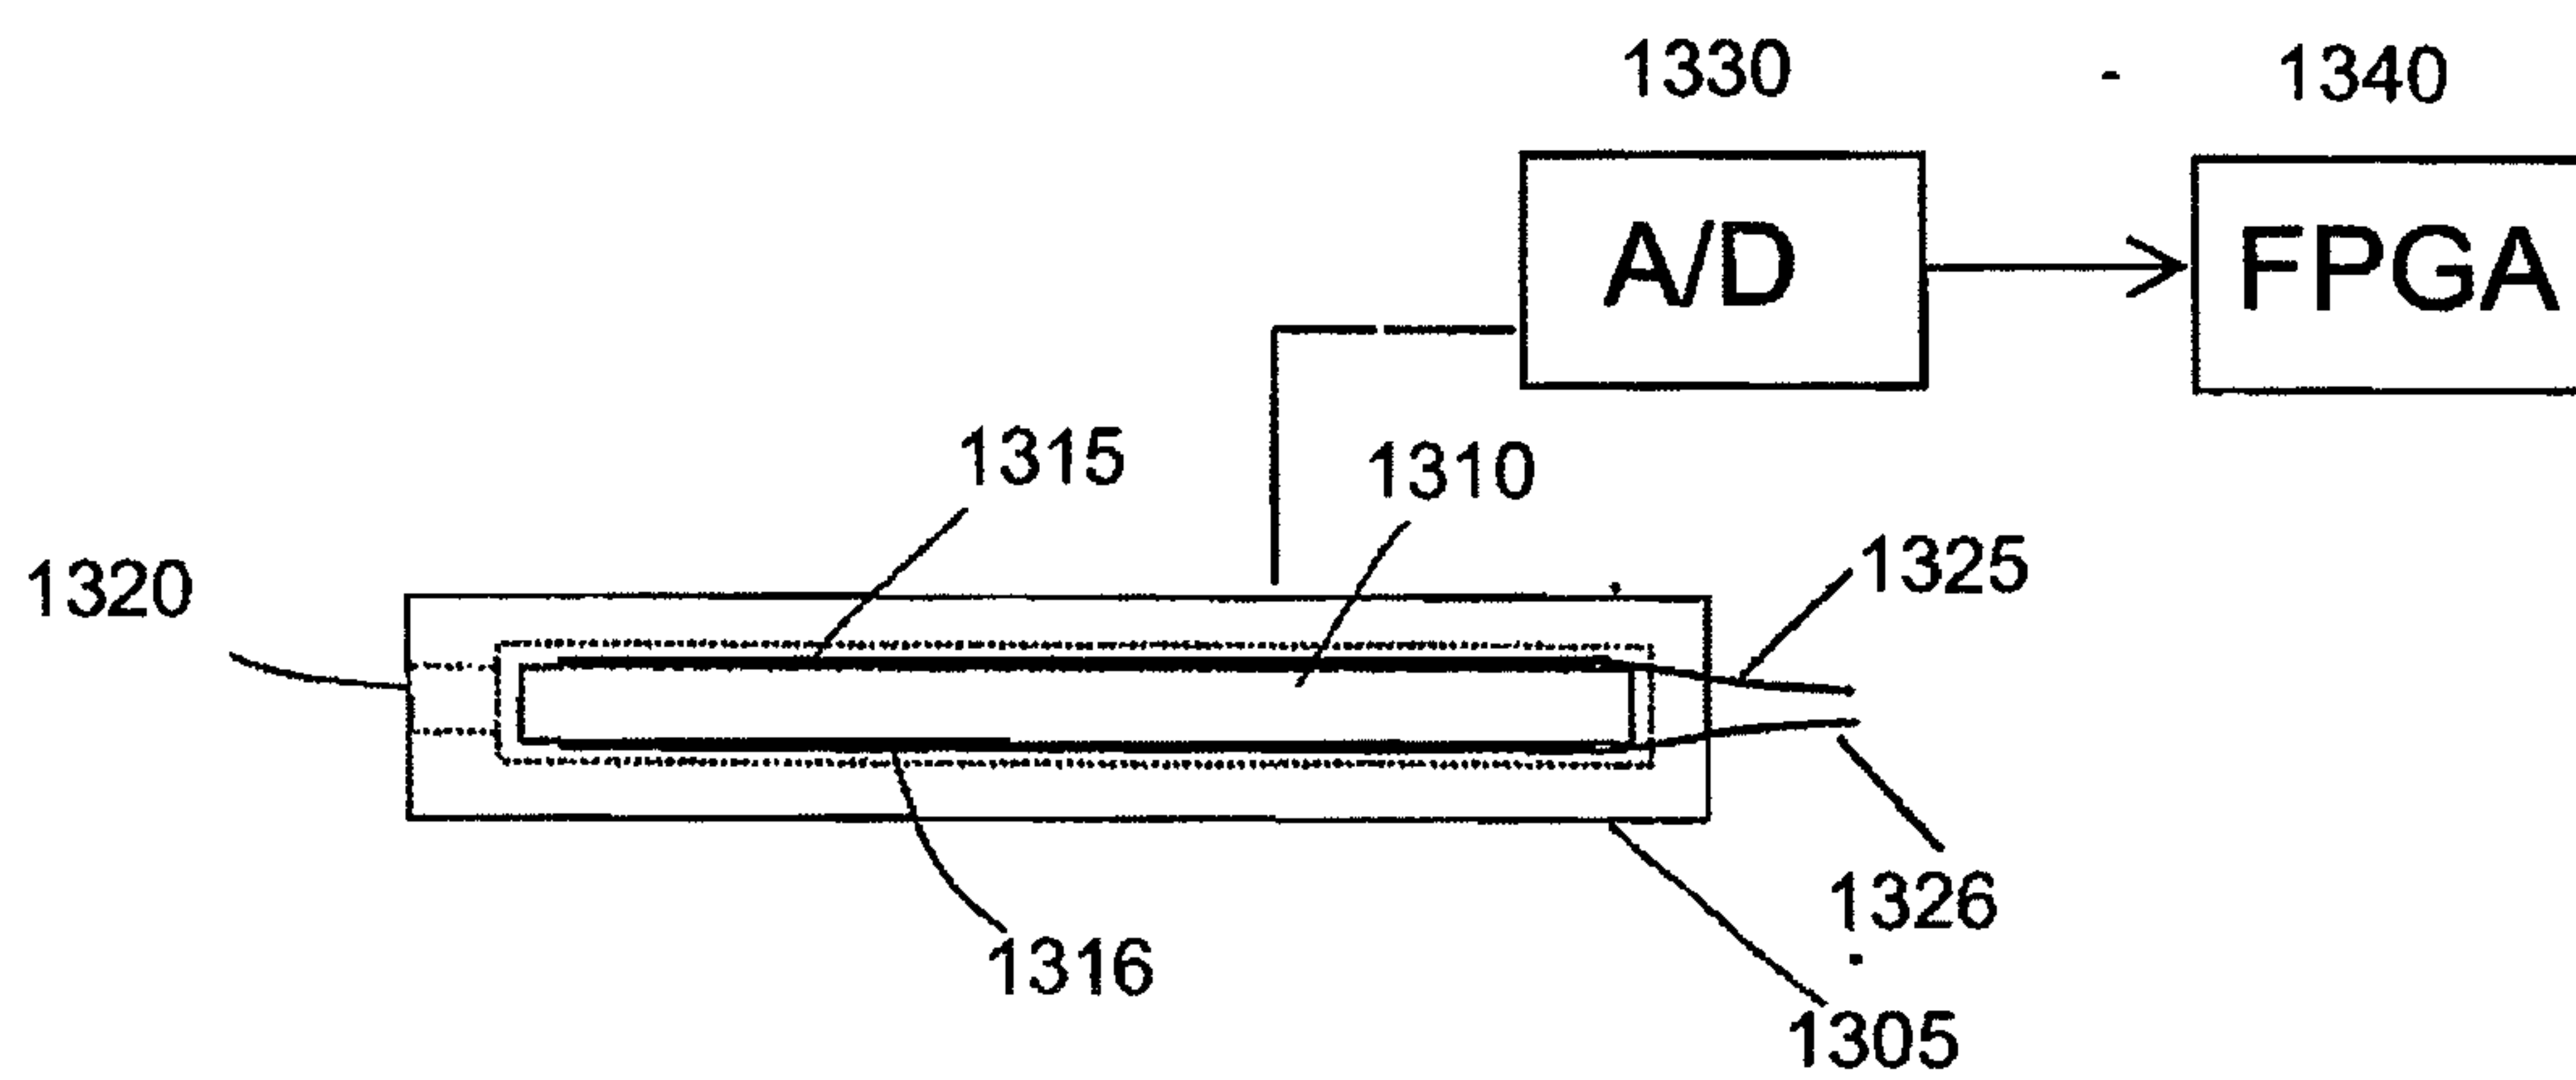


FIG. 14



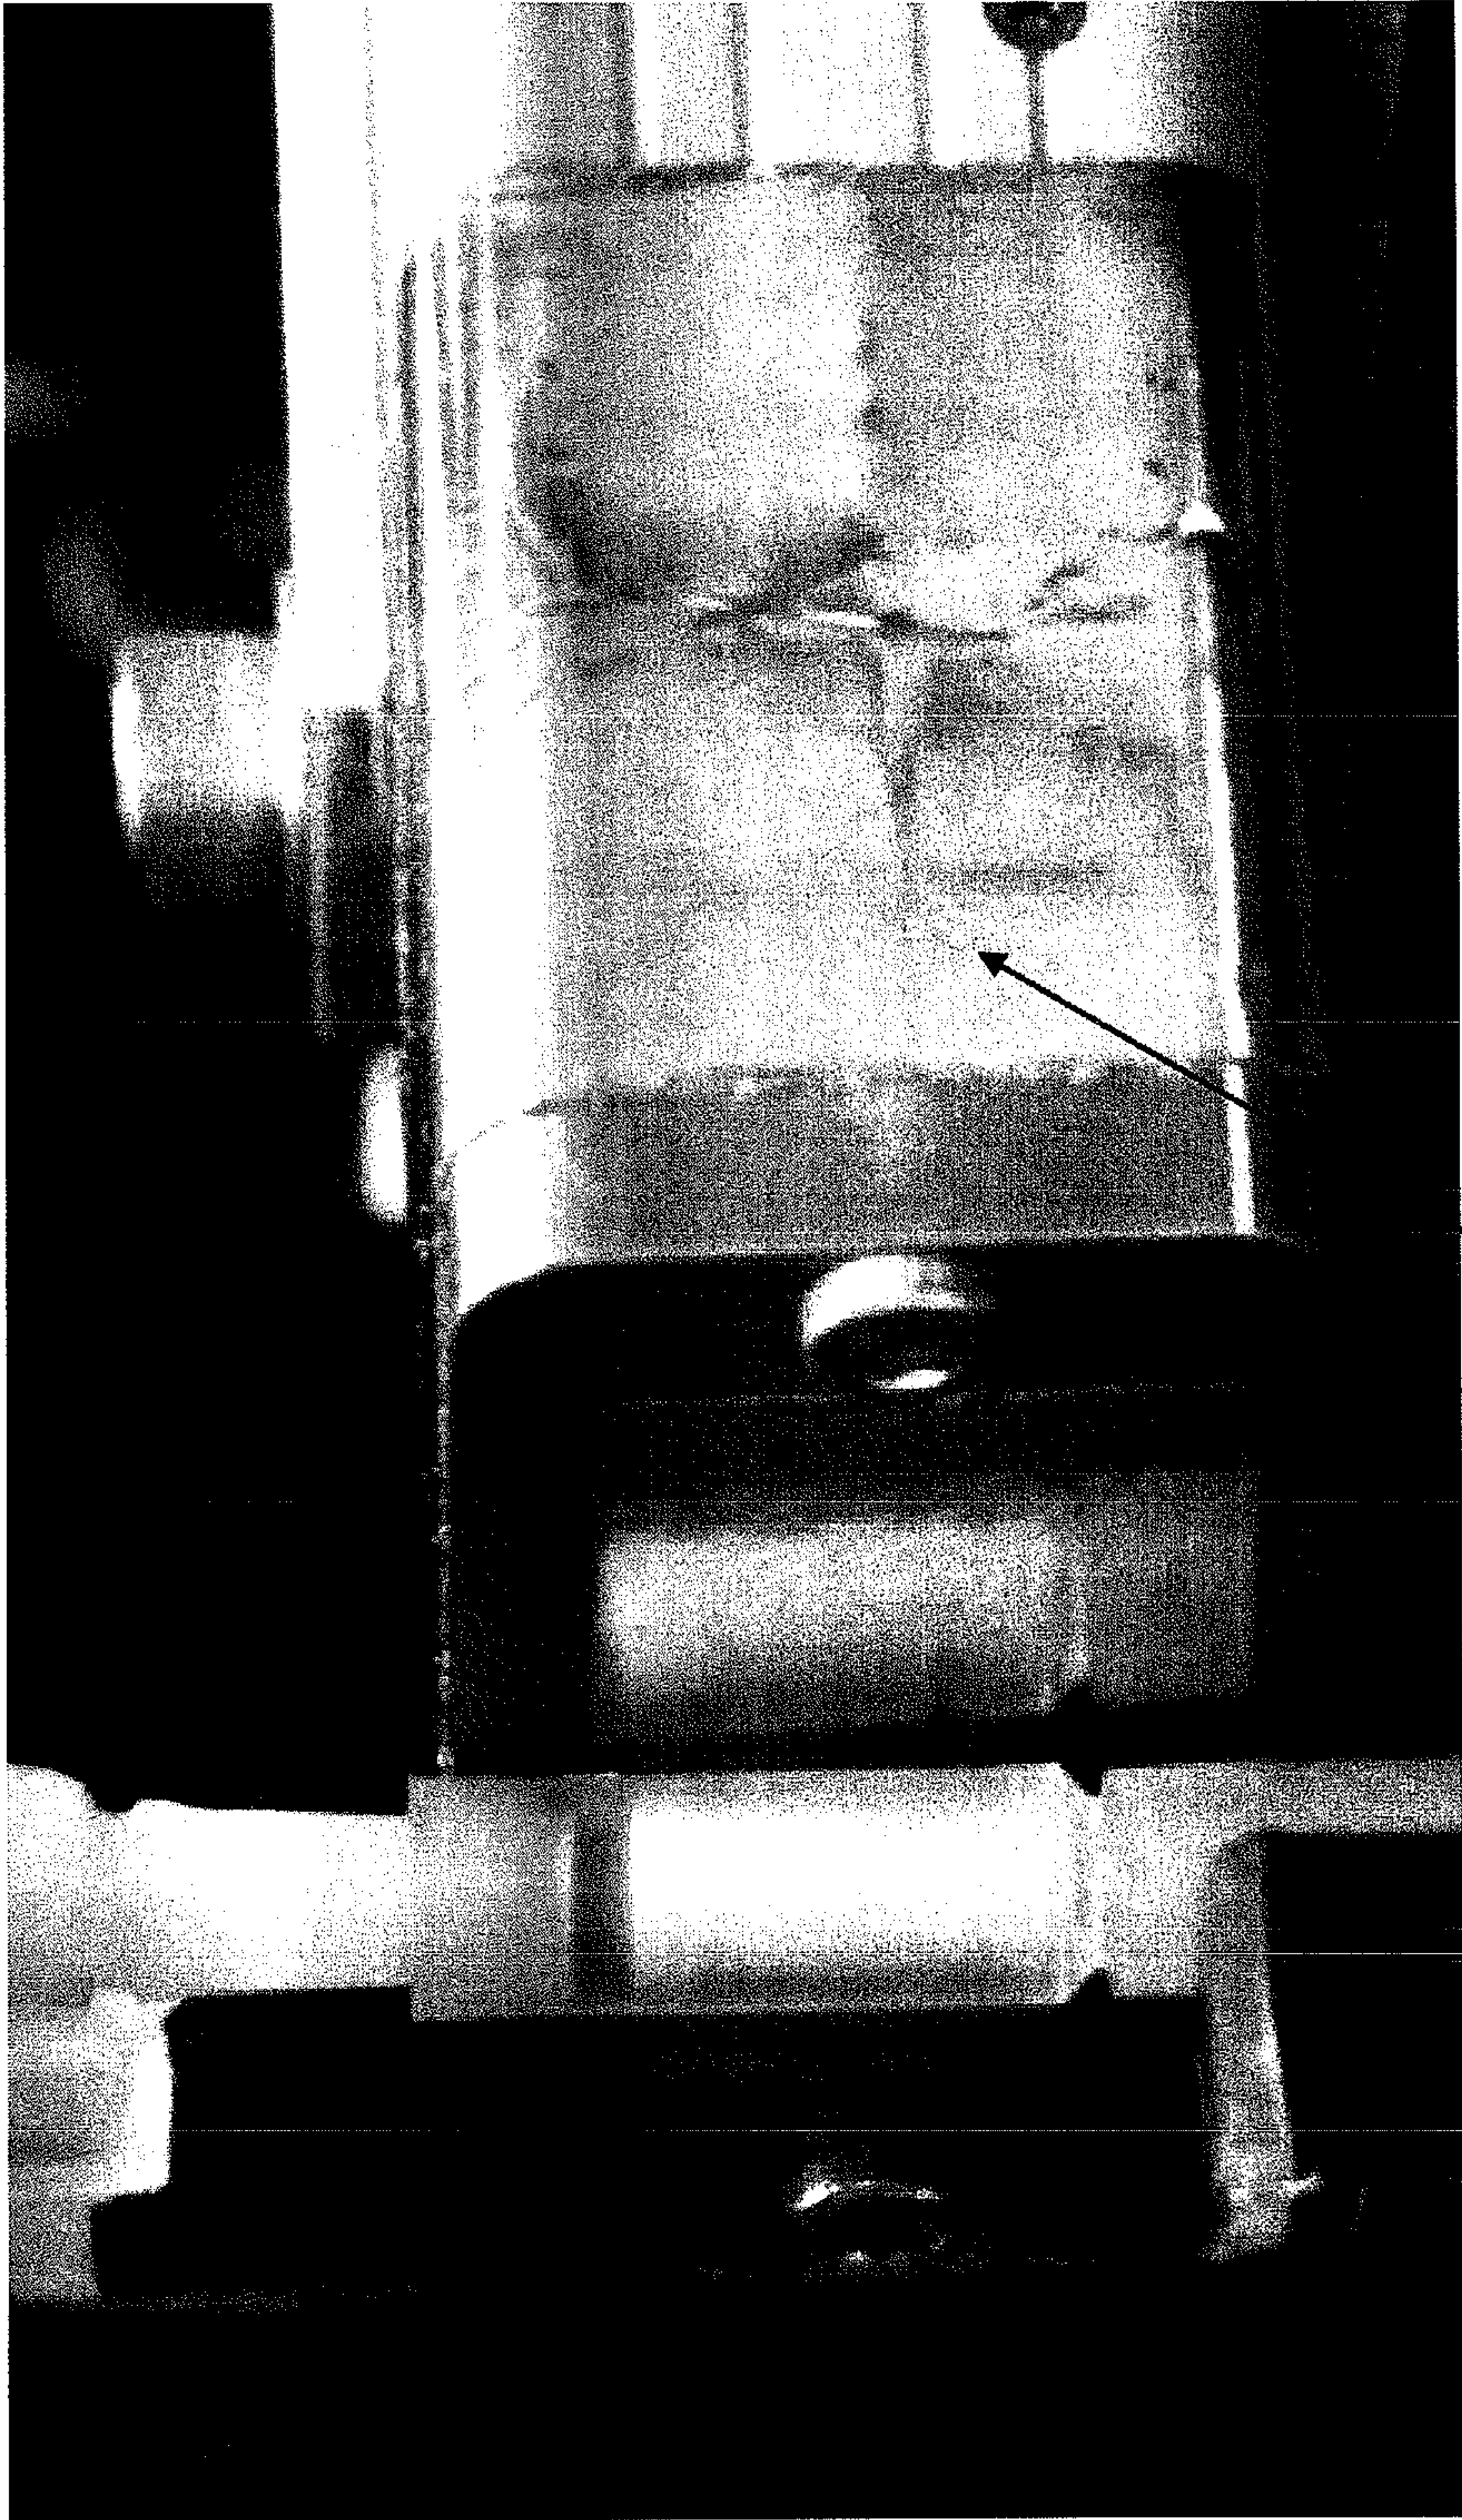


FIG. 15

1500



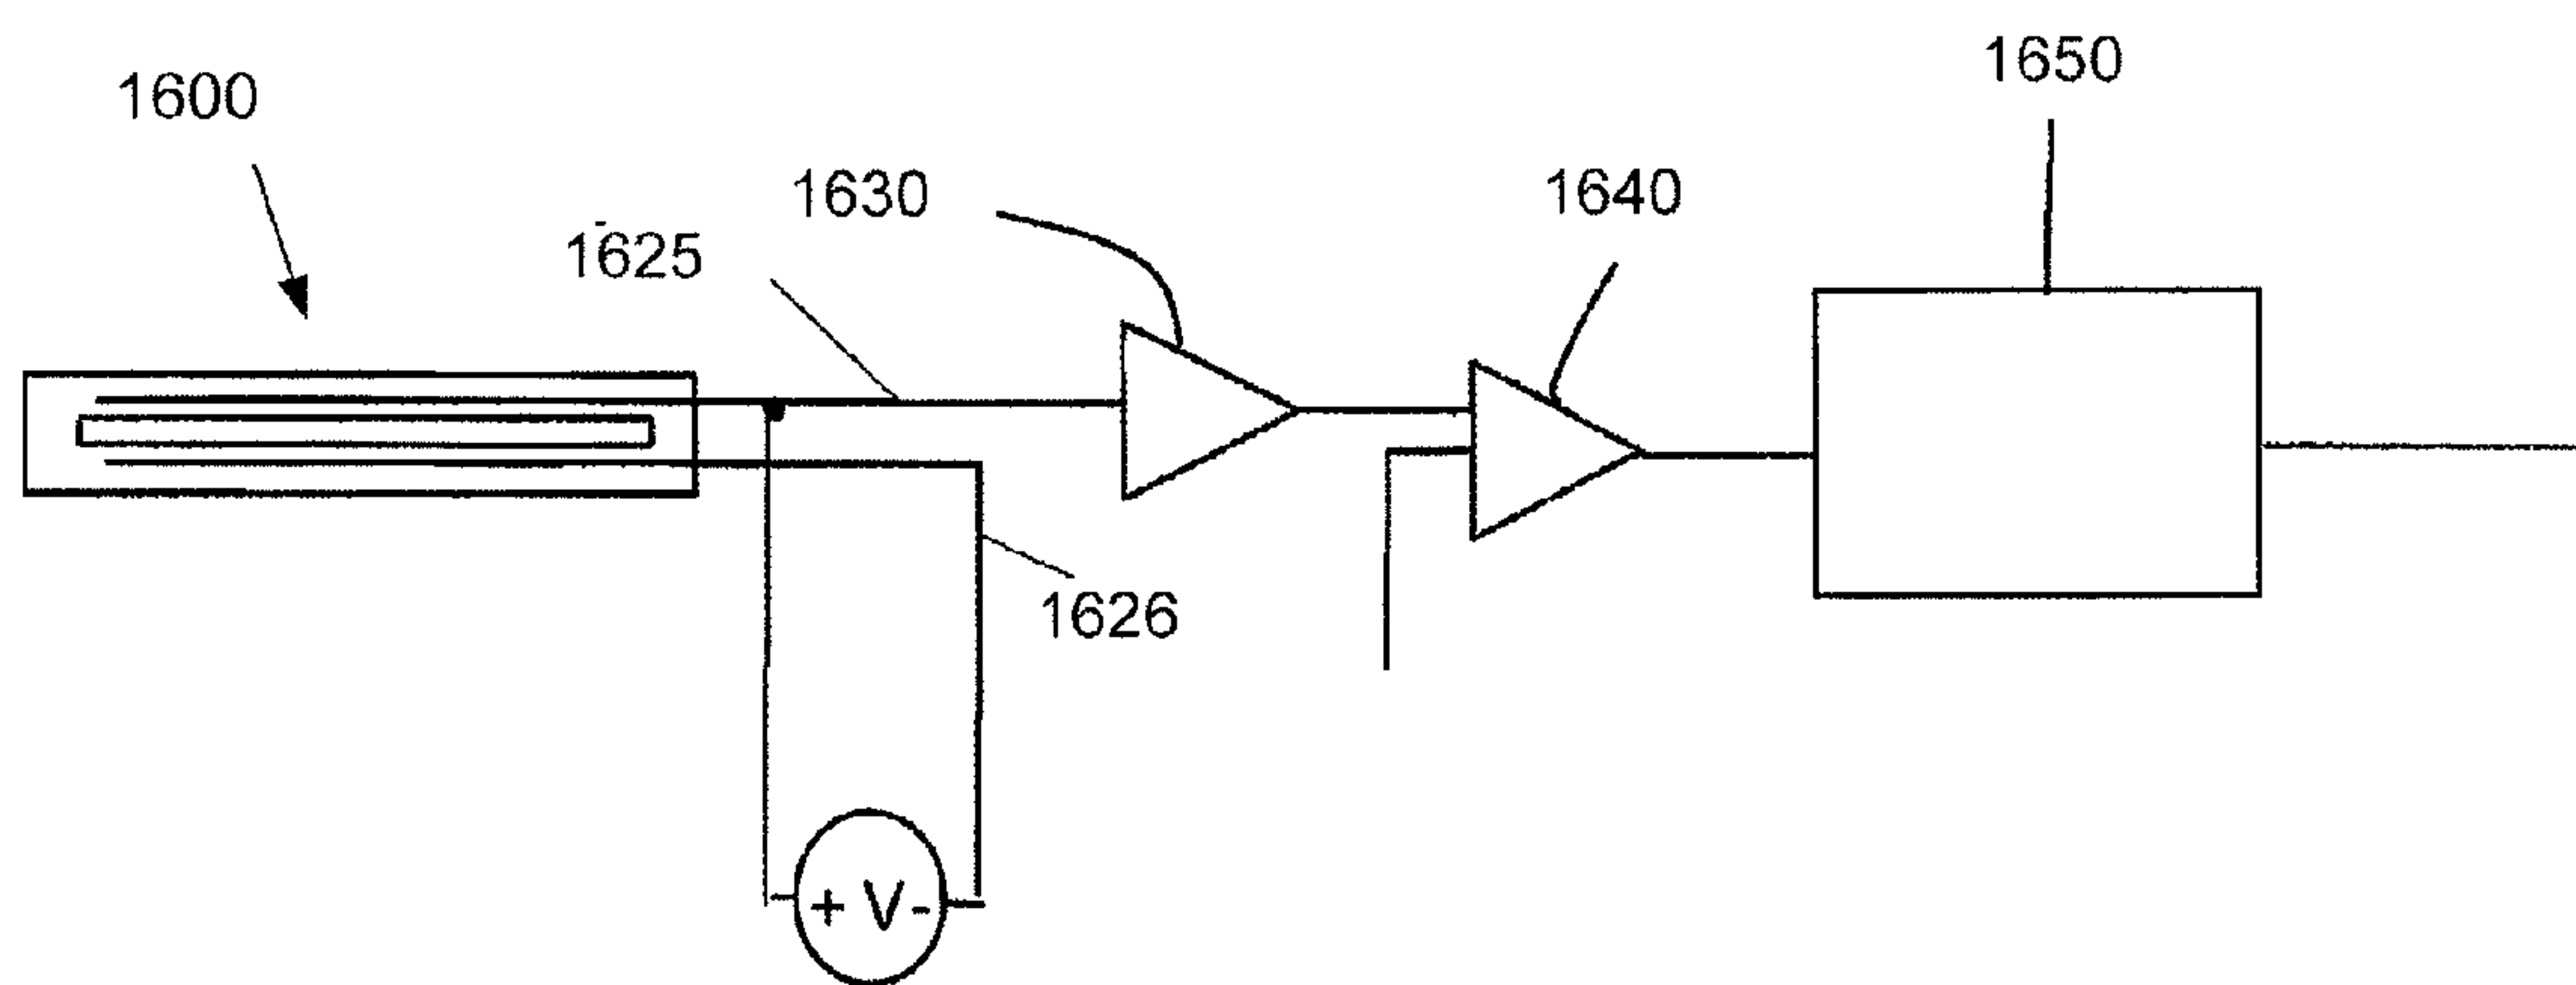


FIG. 16



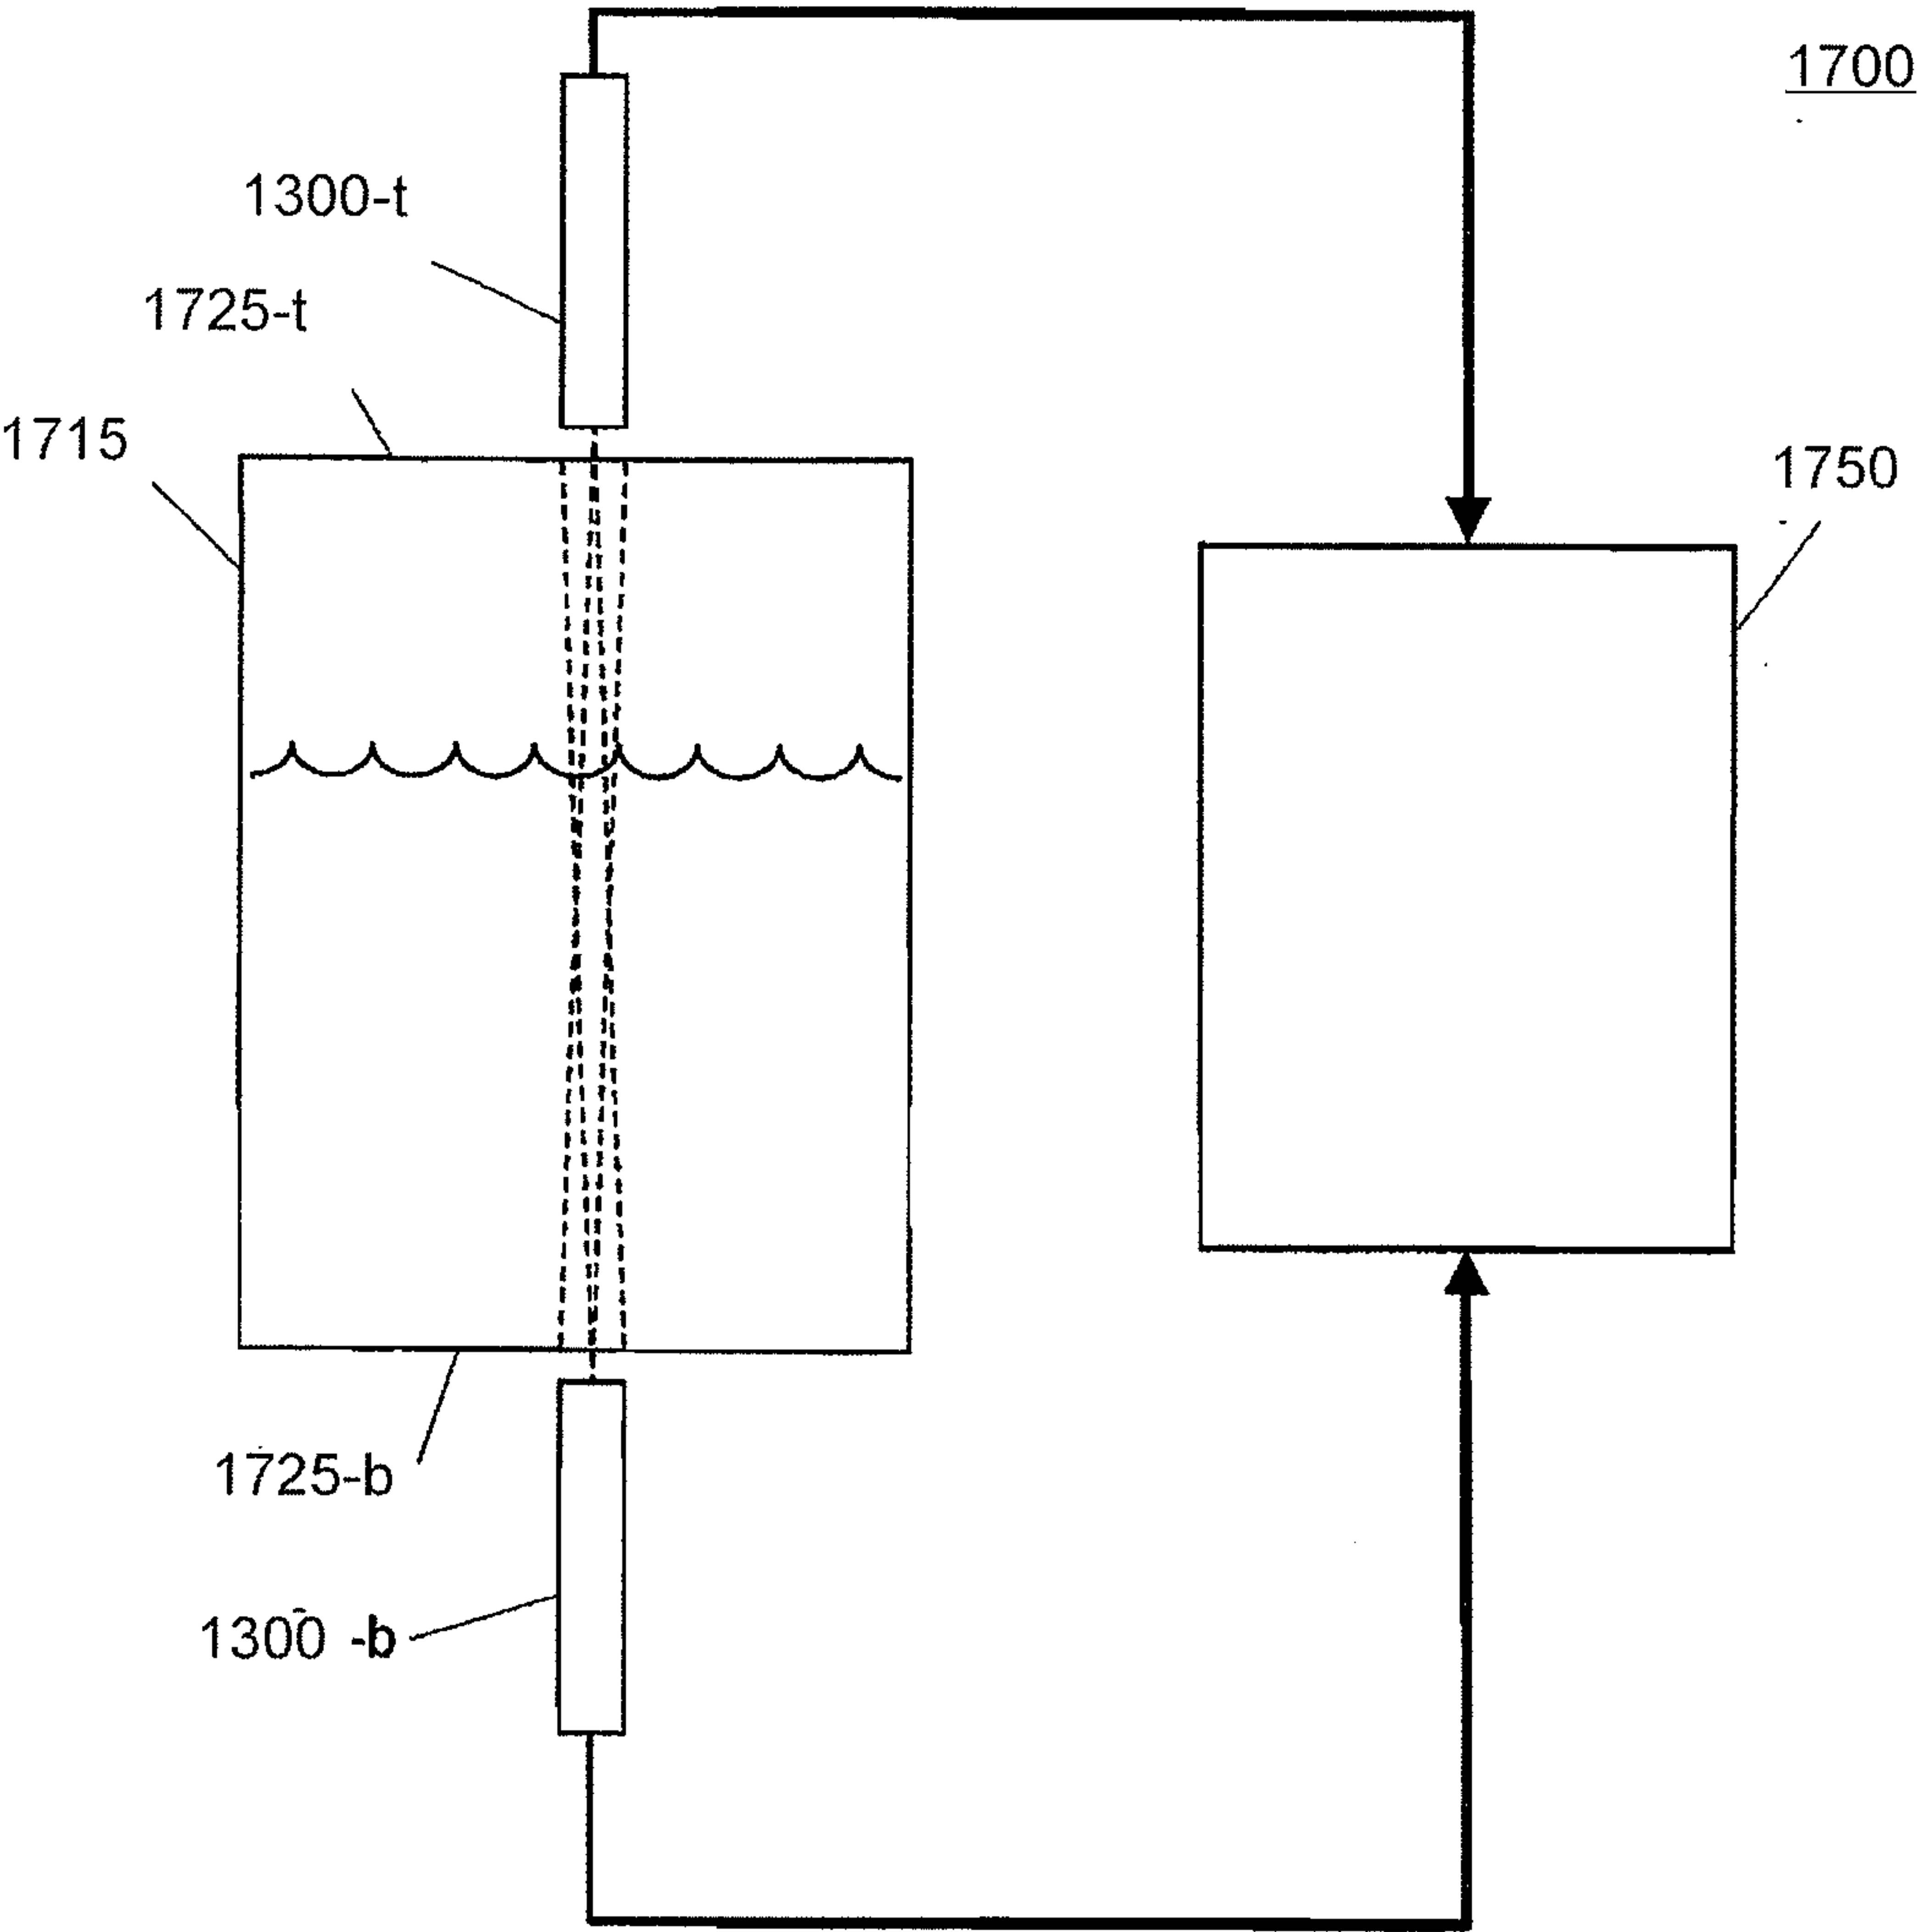


FIG. 17



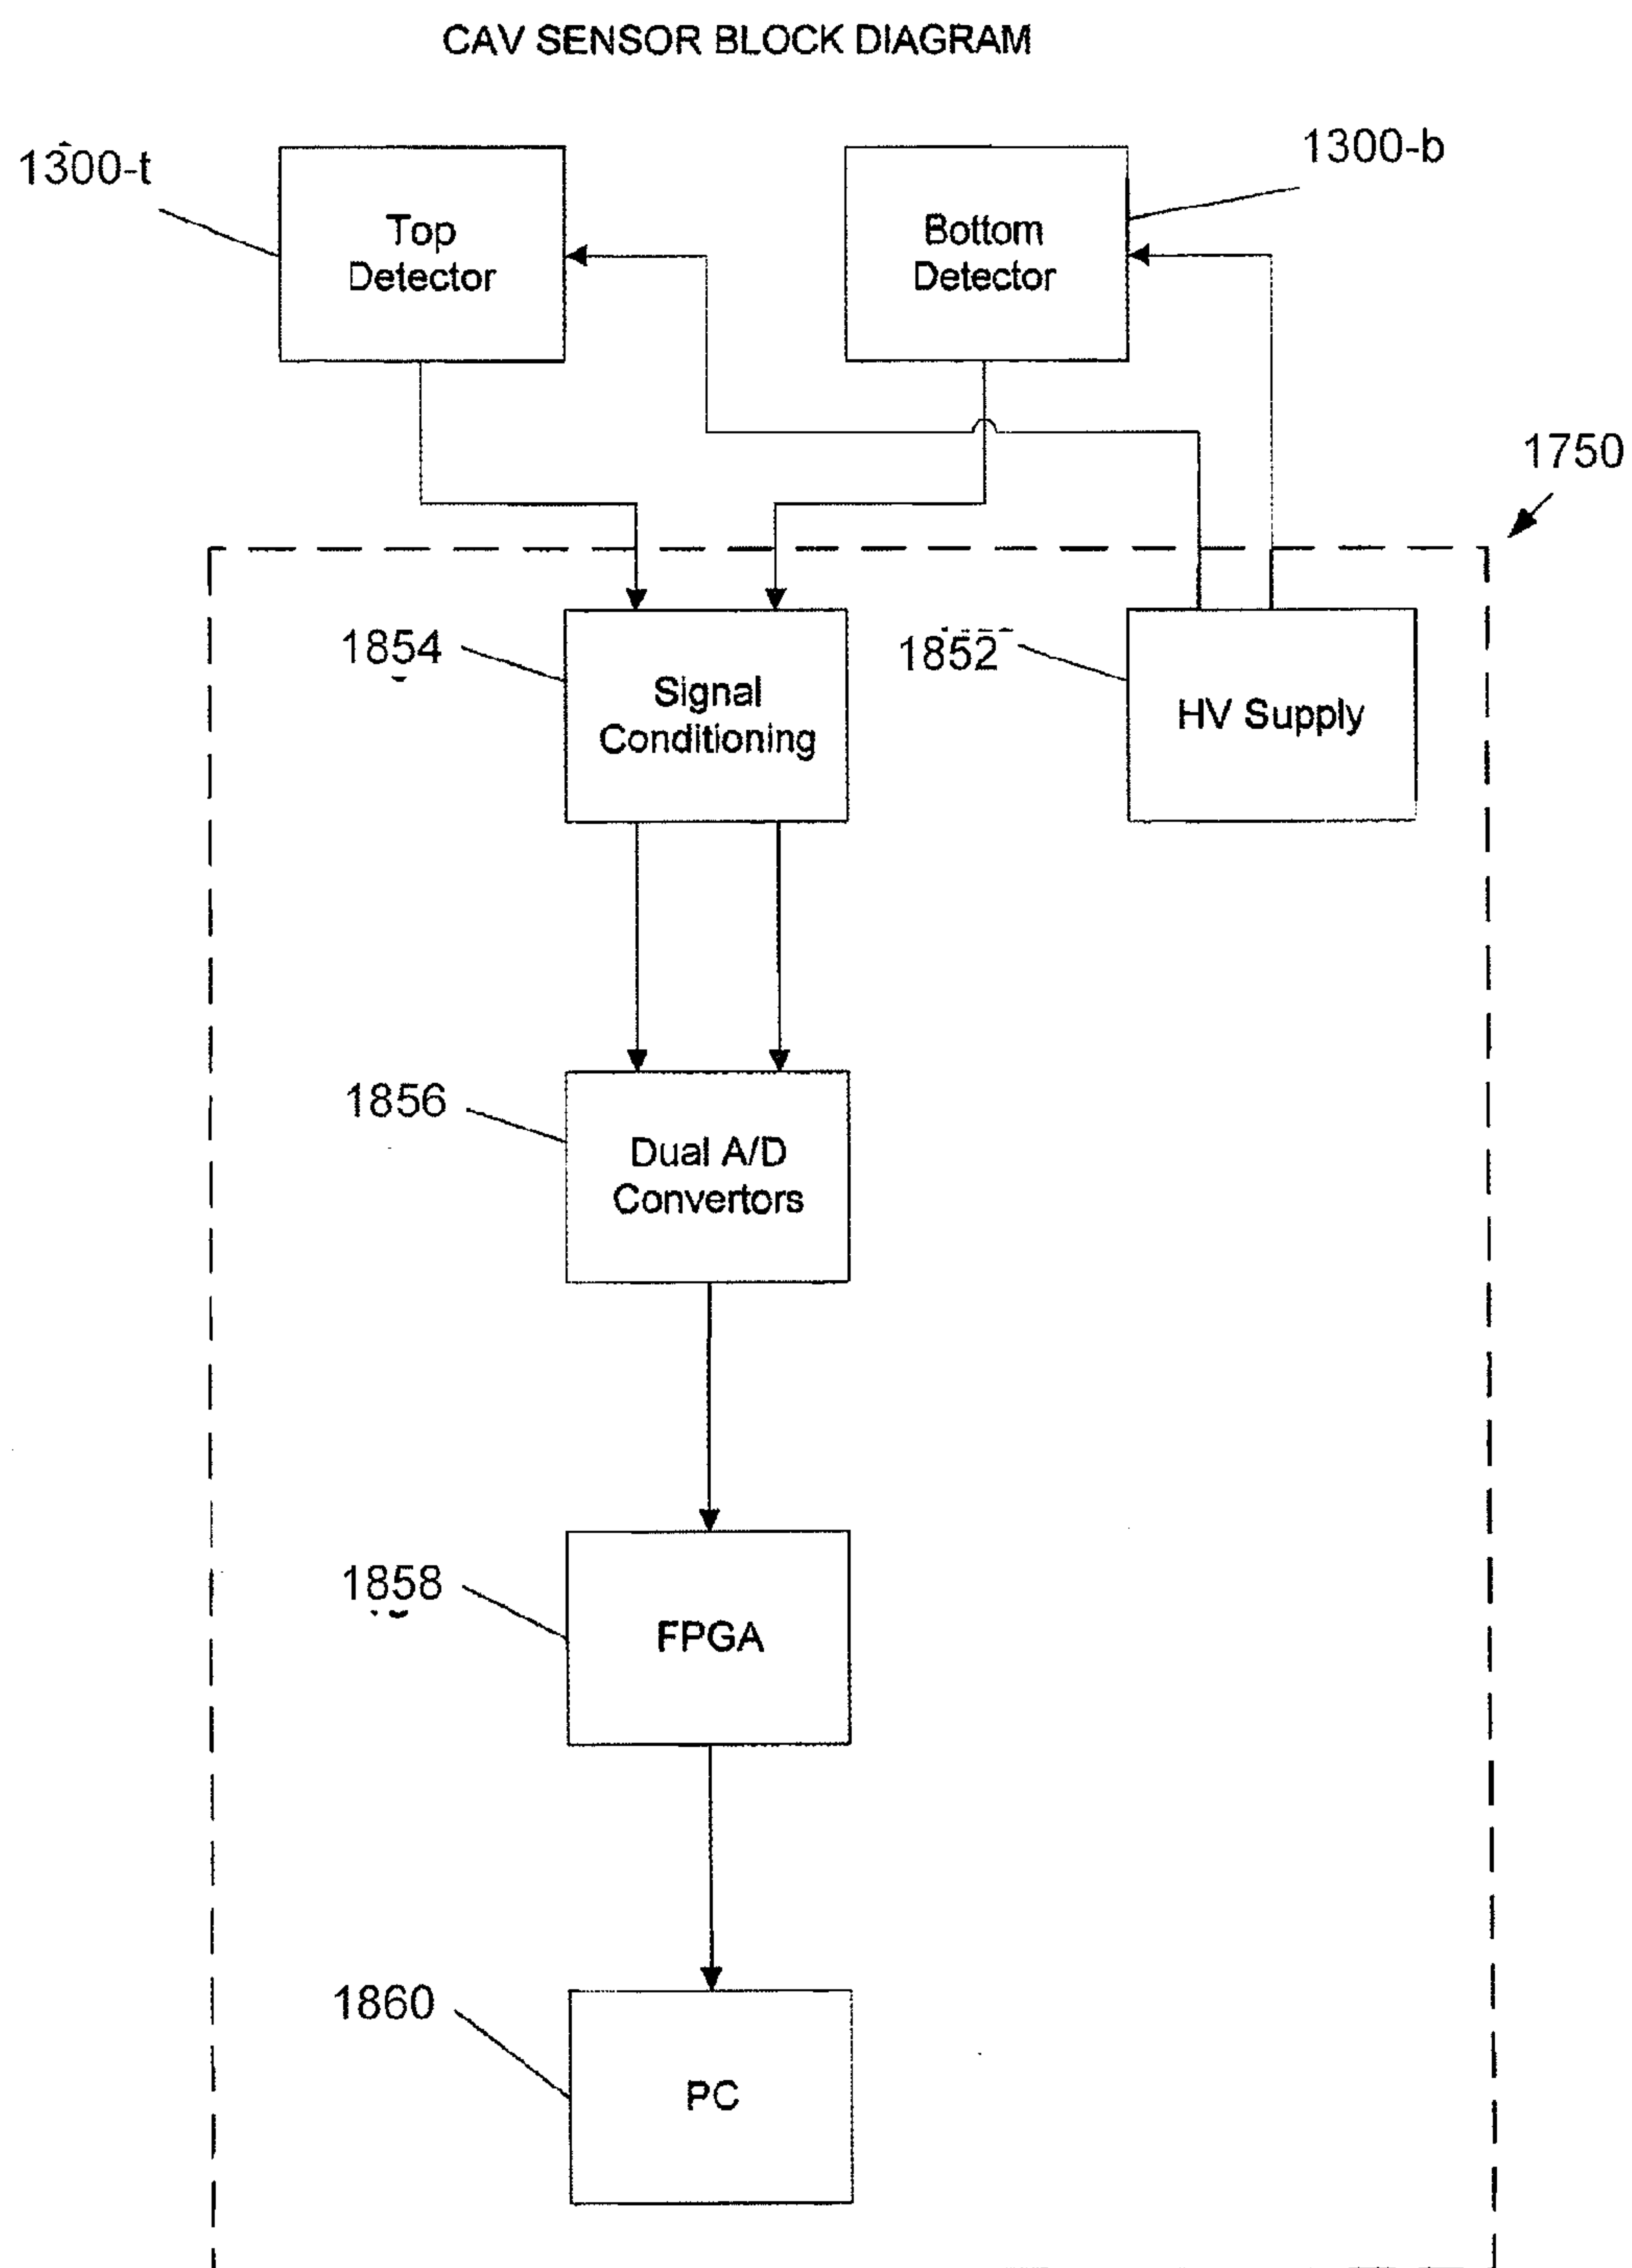


FIG. 18

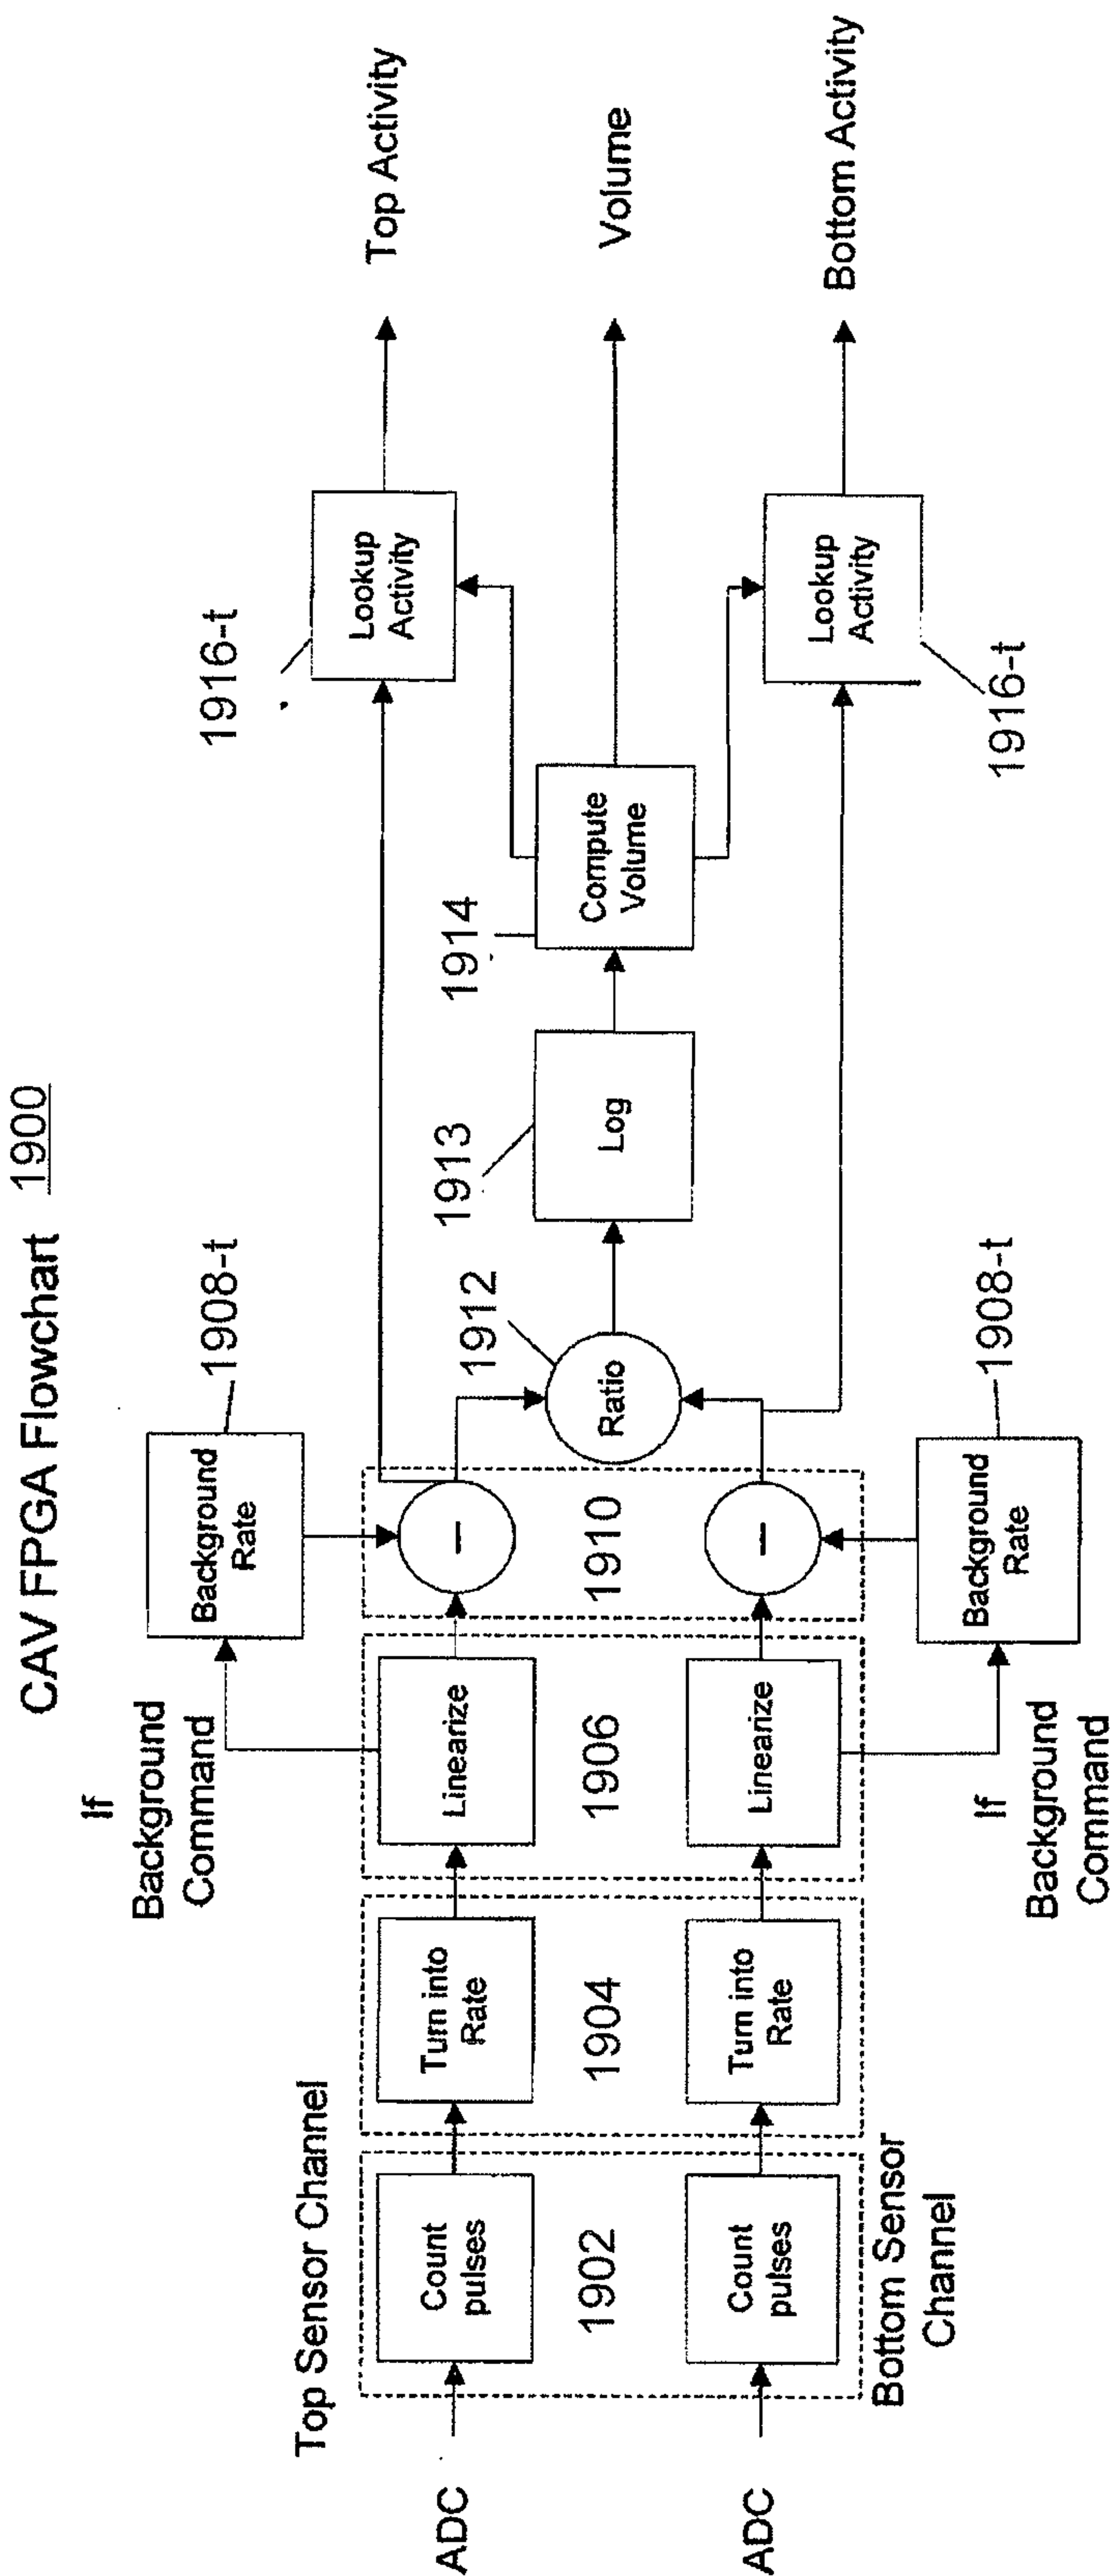


FIG. 19



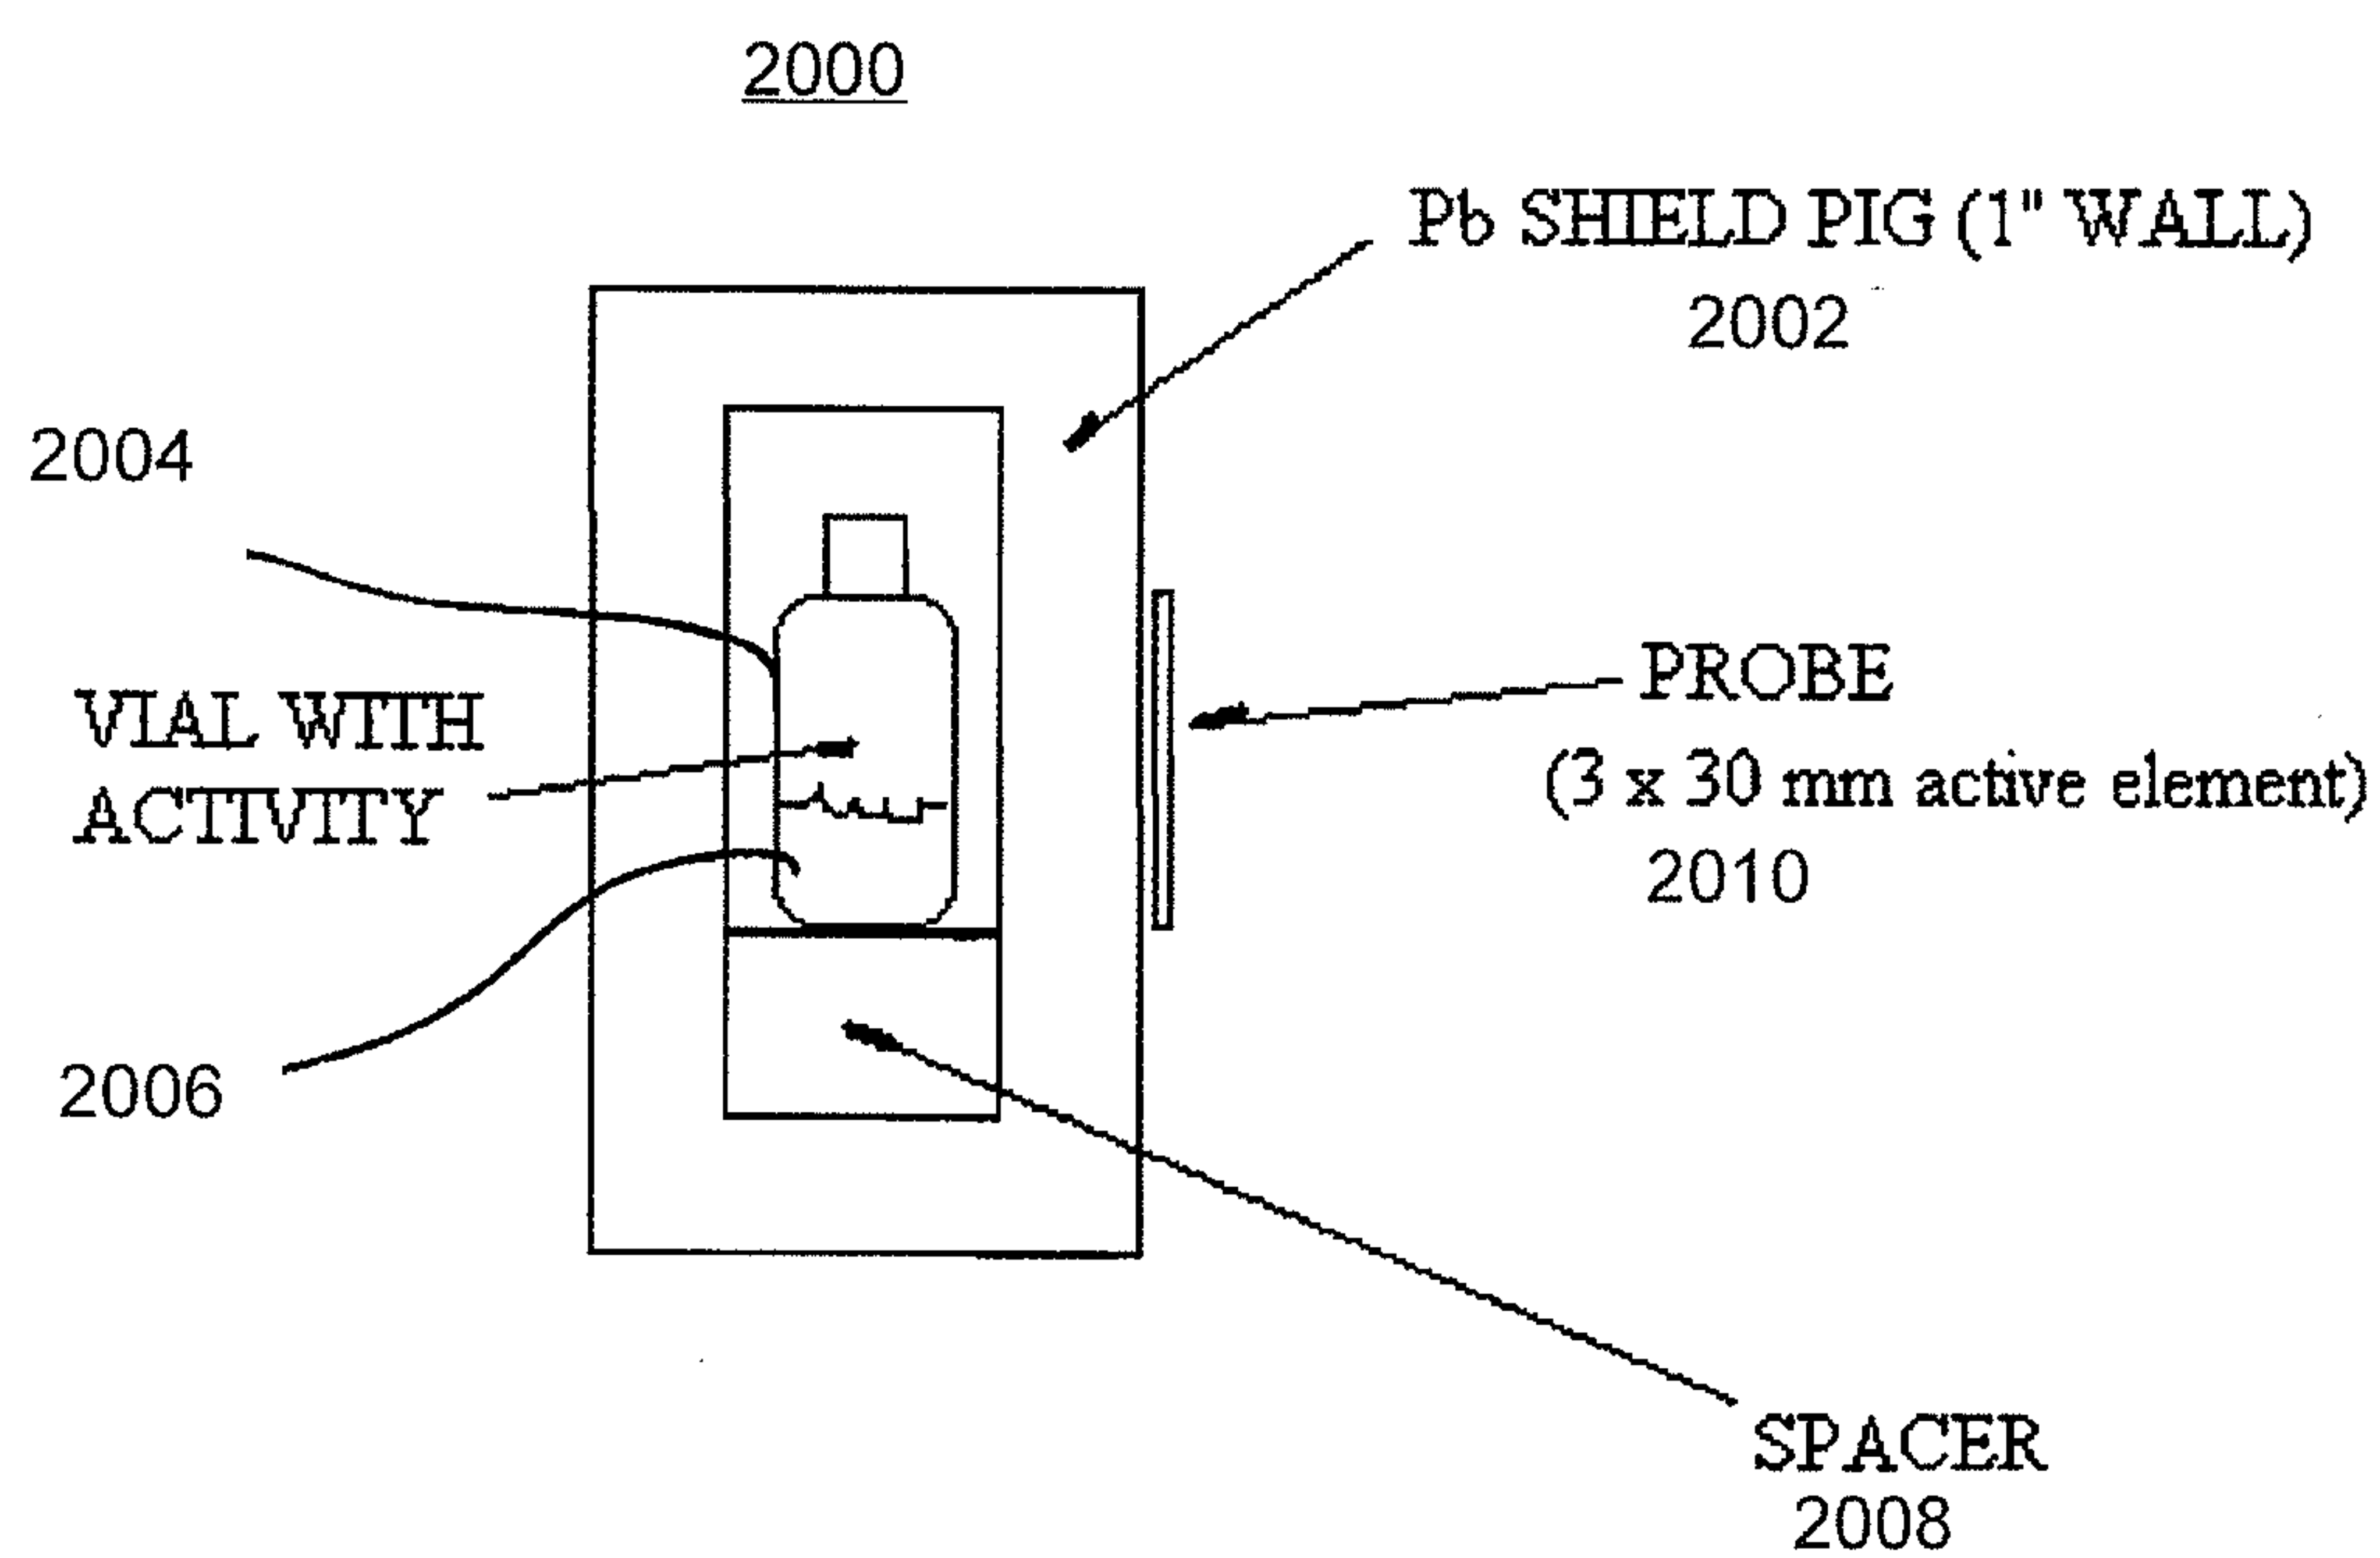


FIG. 20

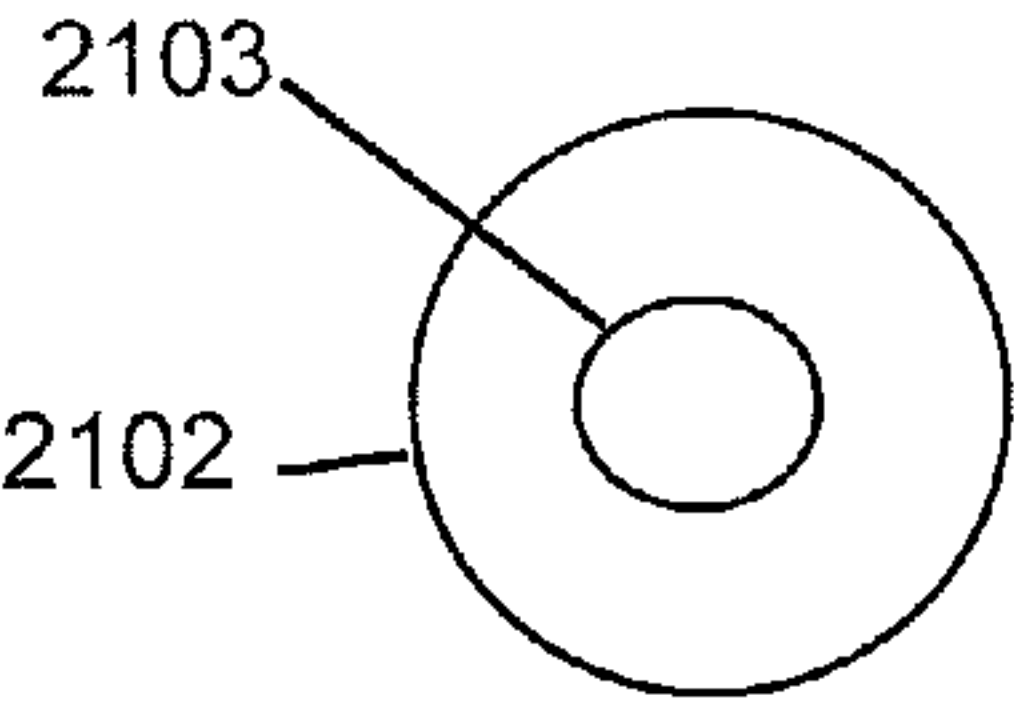
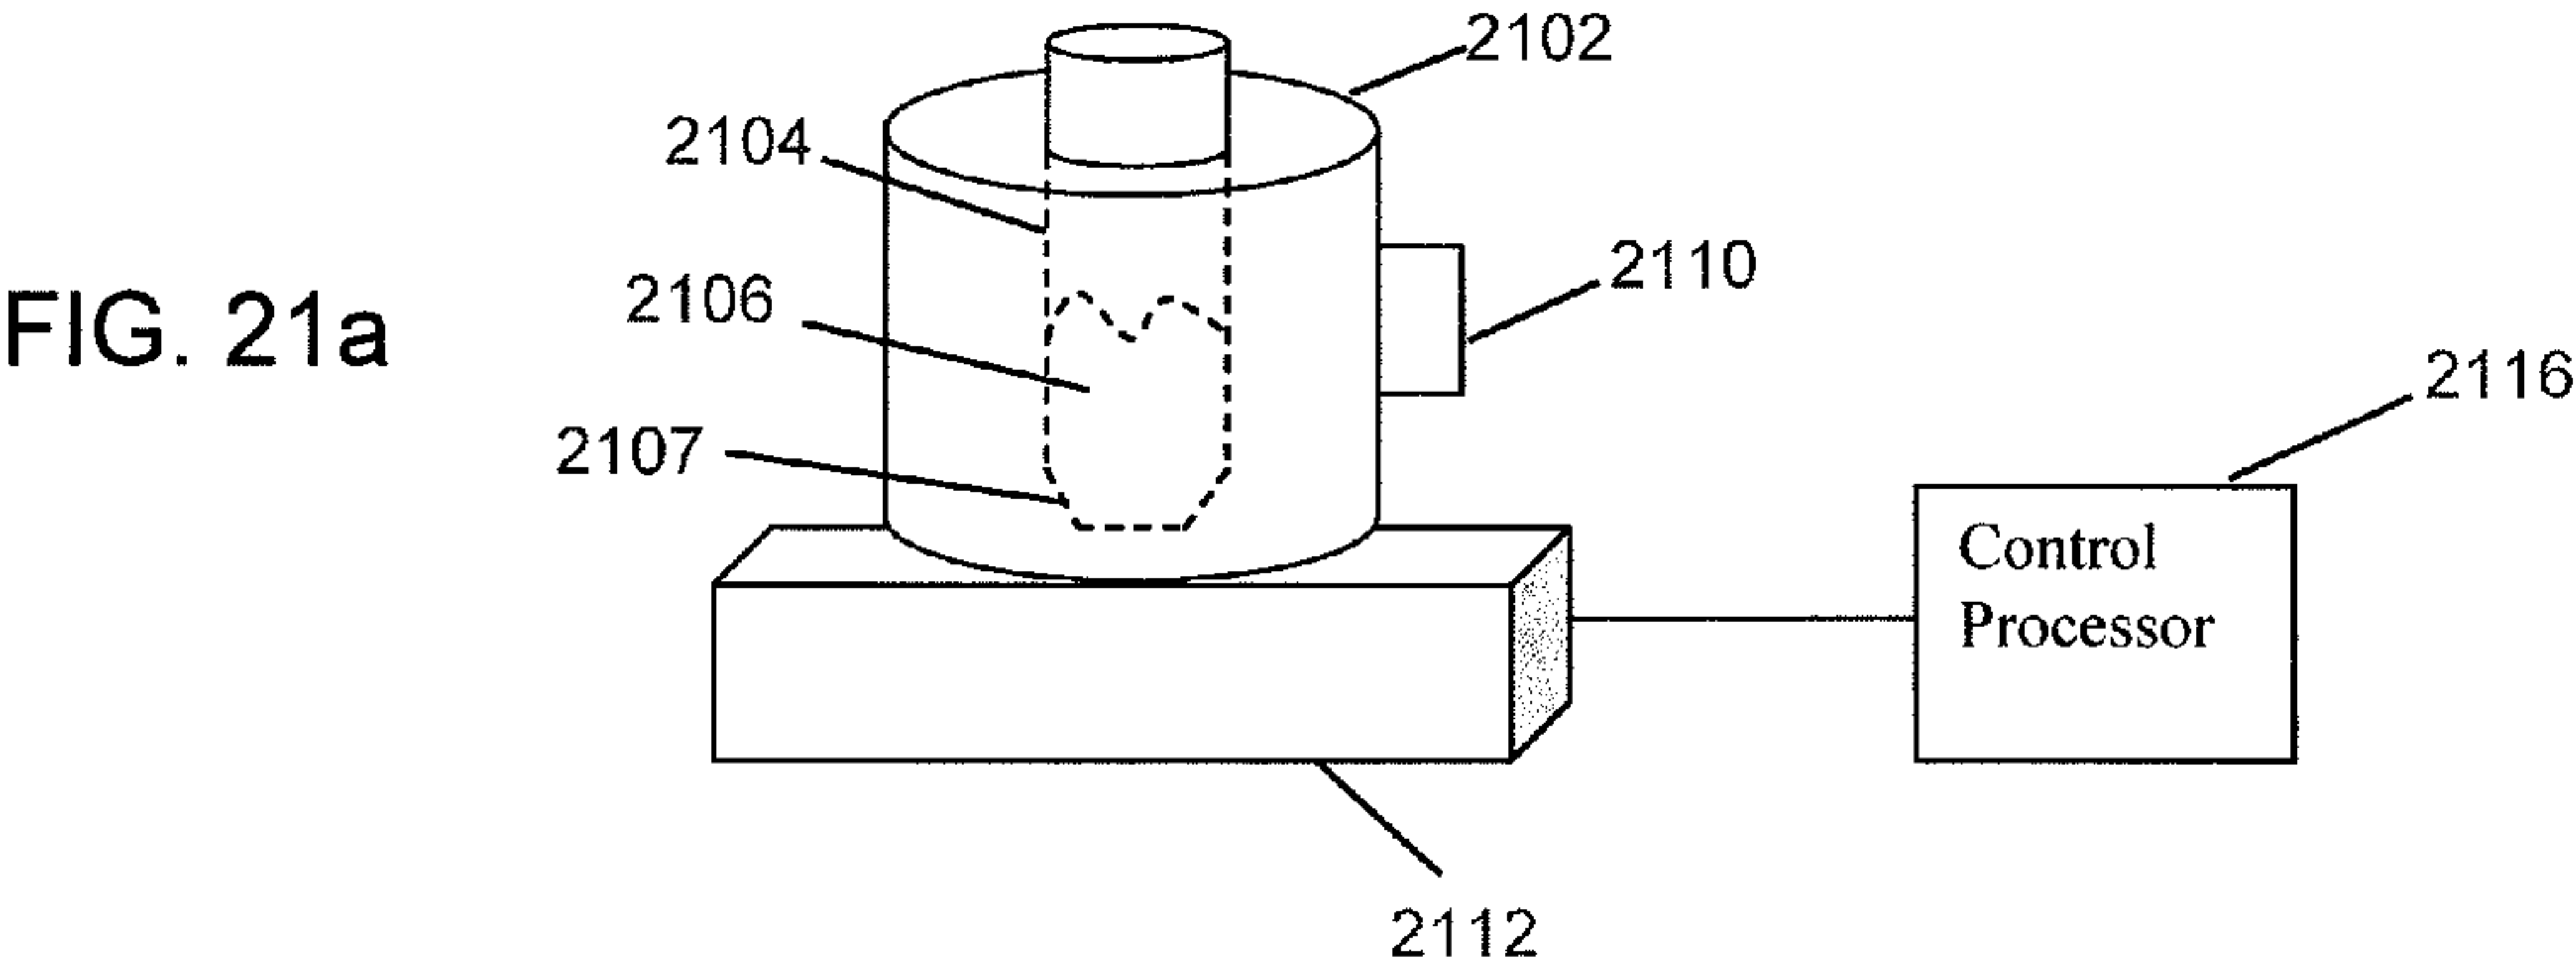


FIG. 21b

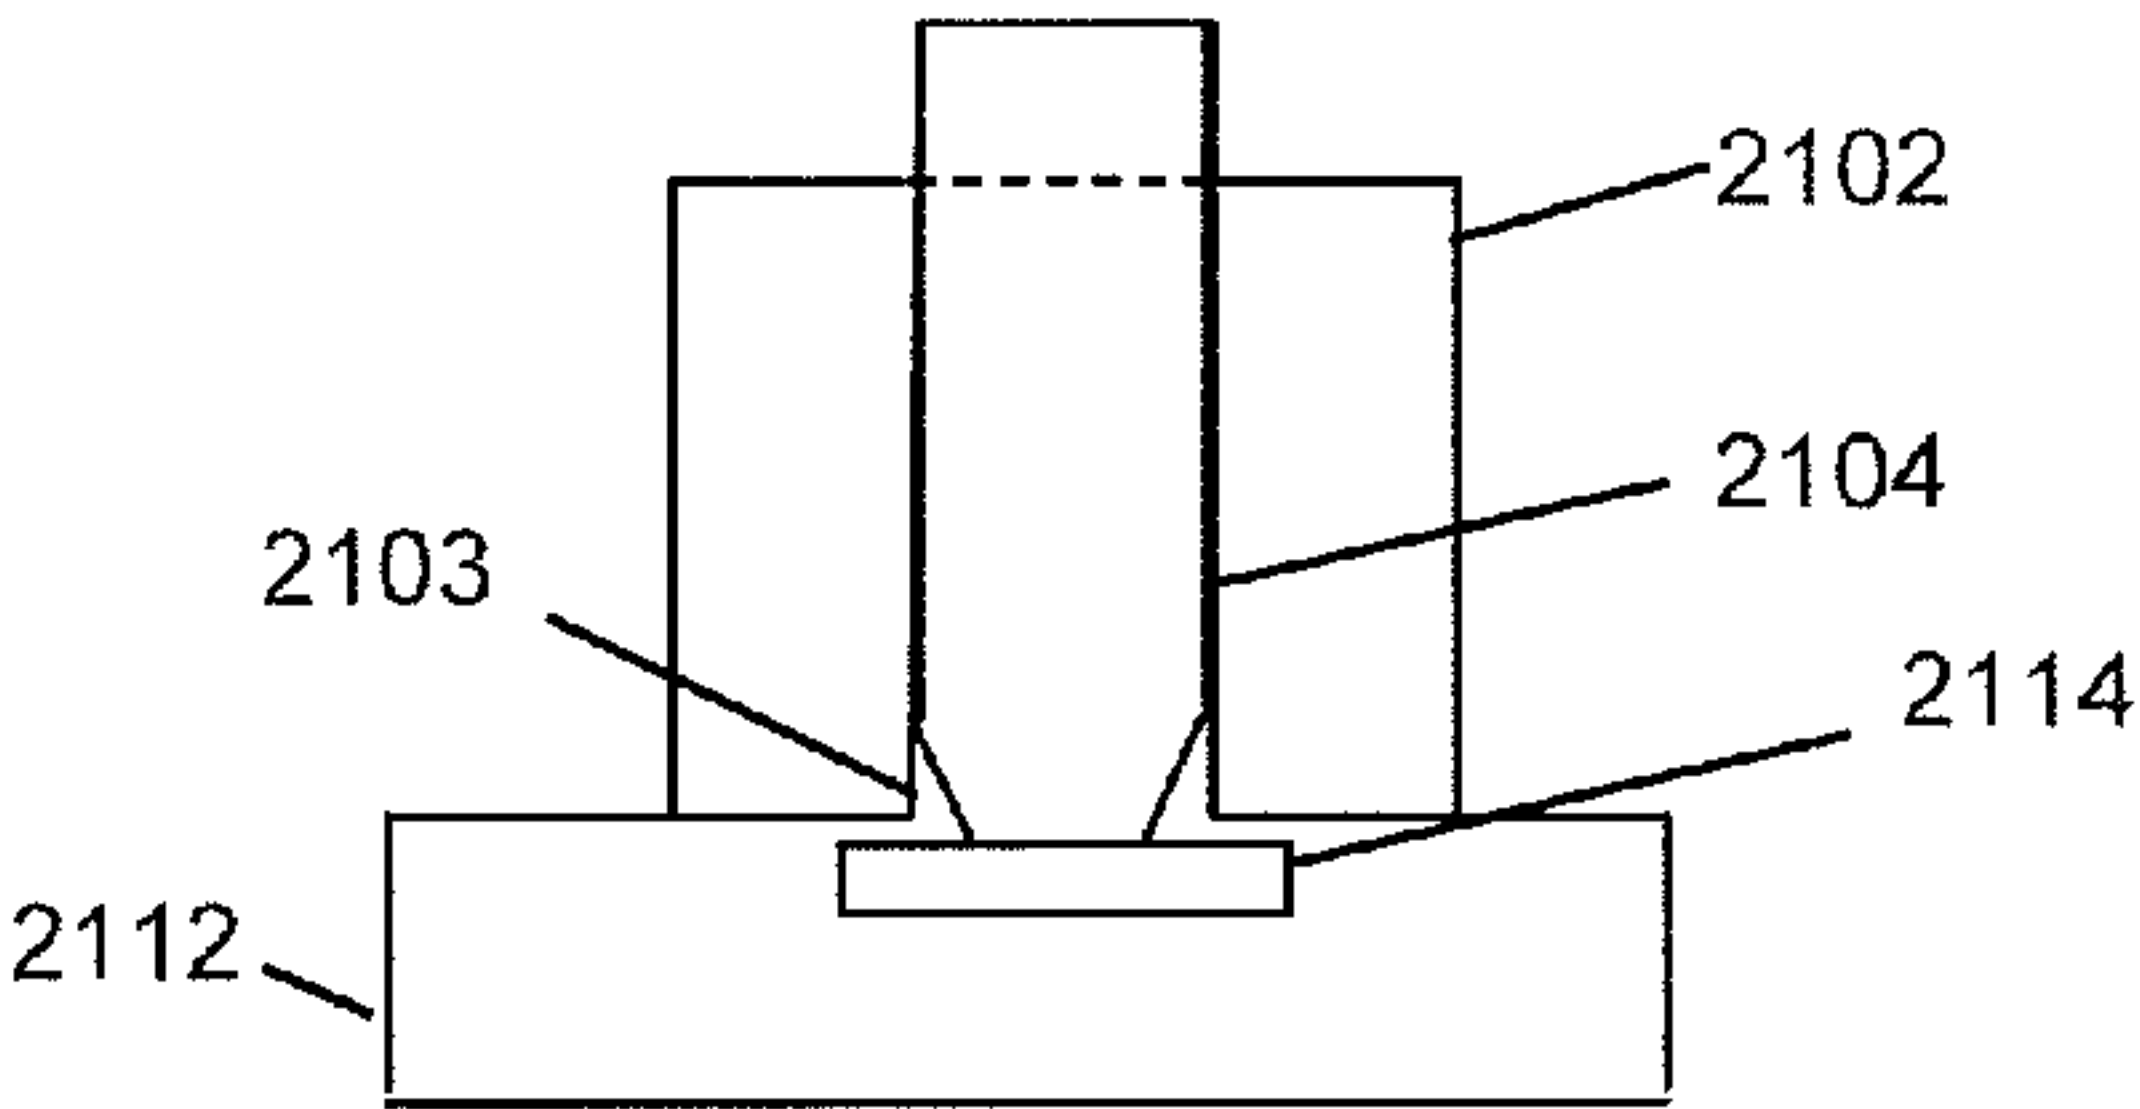


FIG. 21c



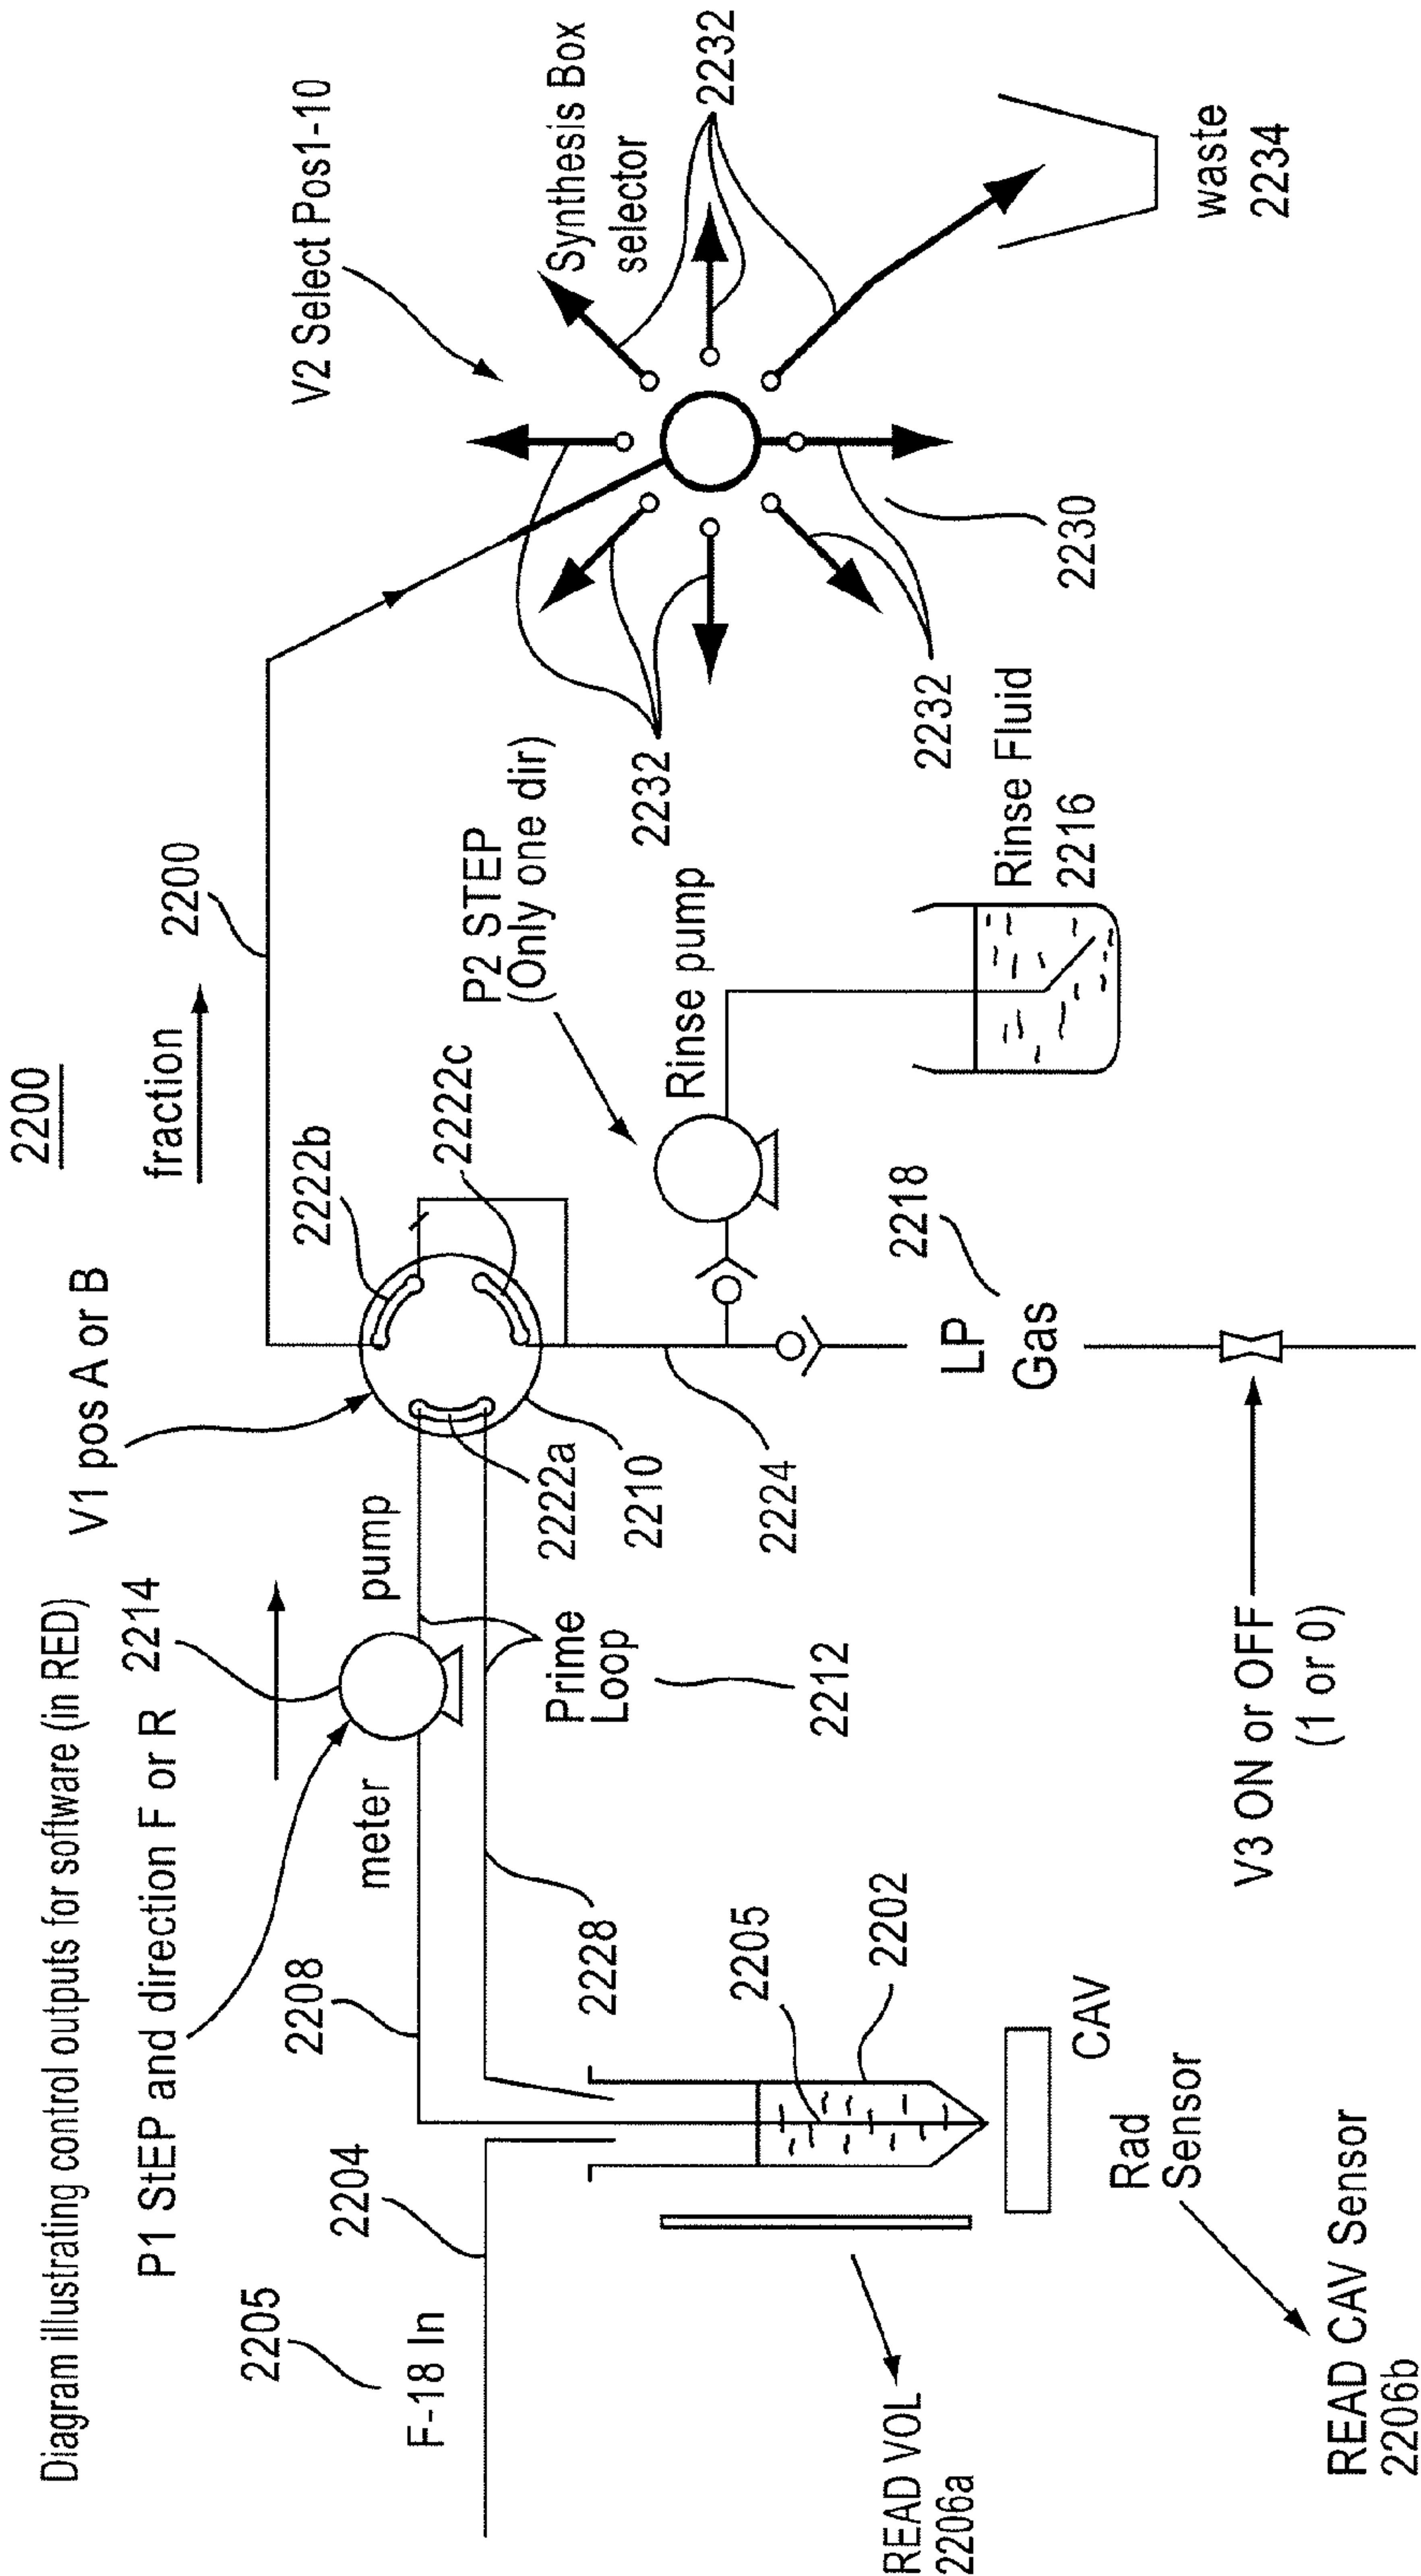


FIG.22


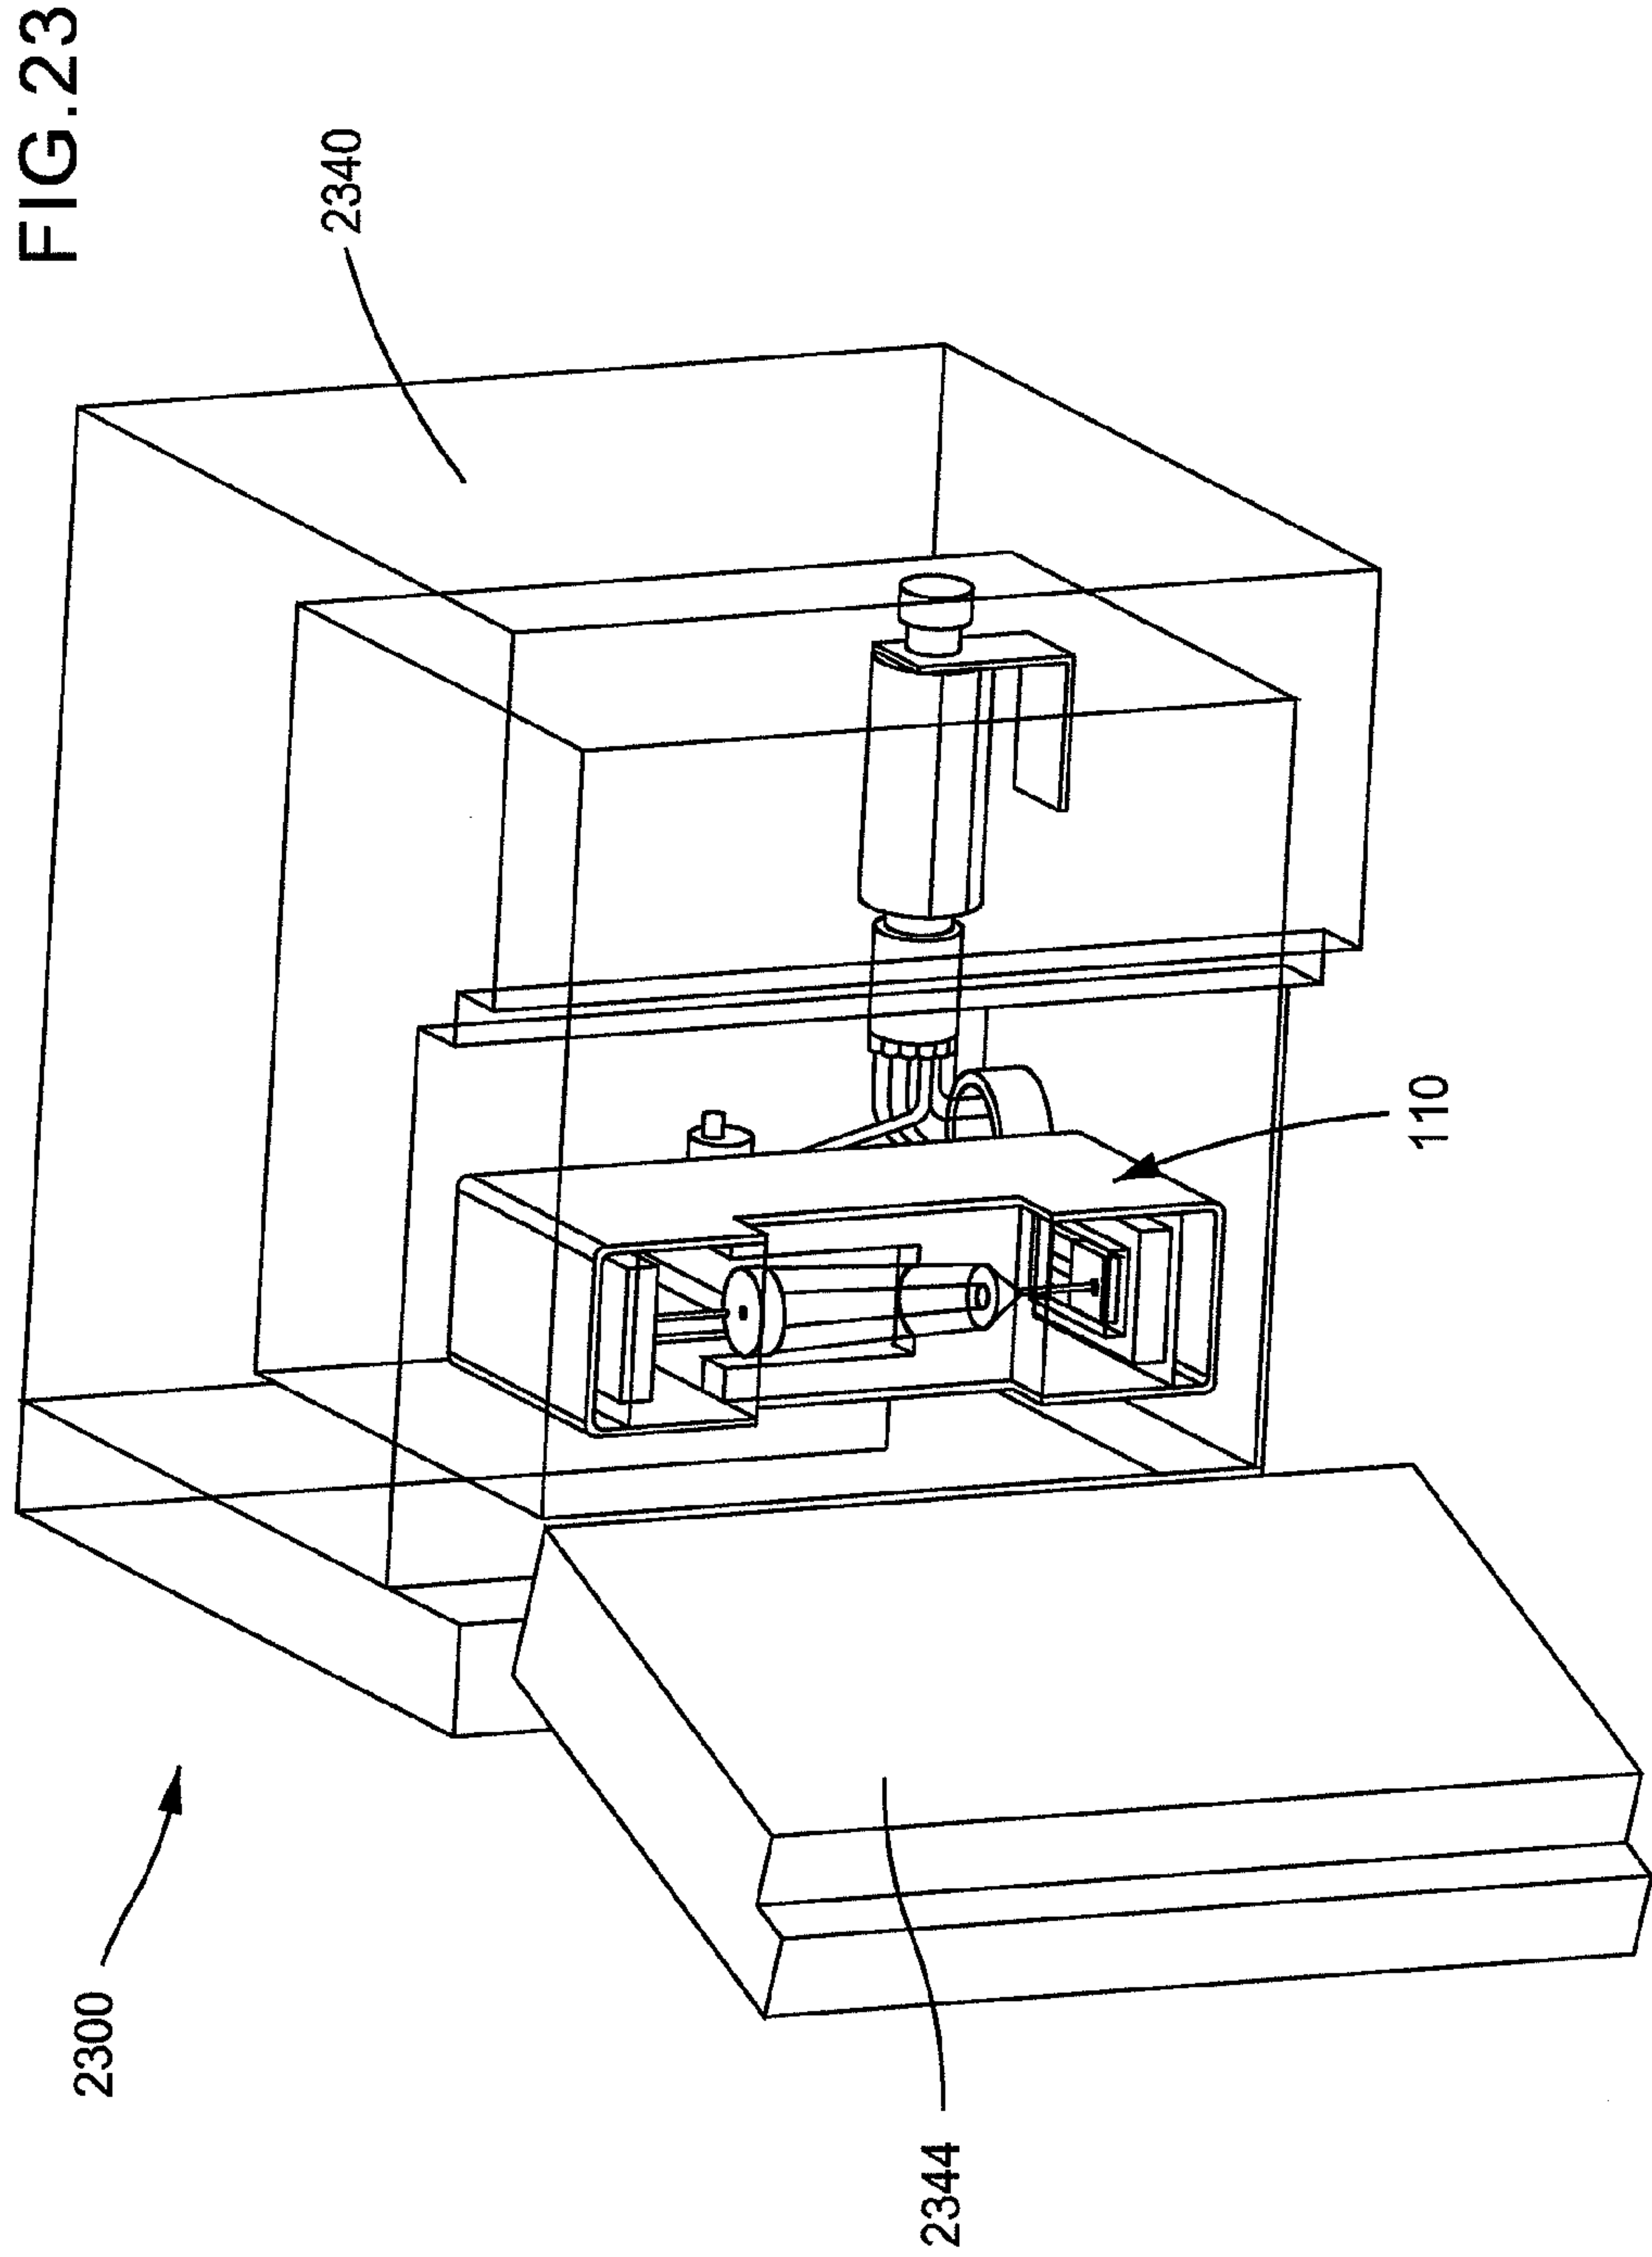




FIG. 24

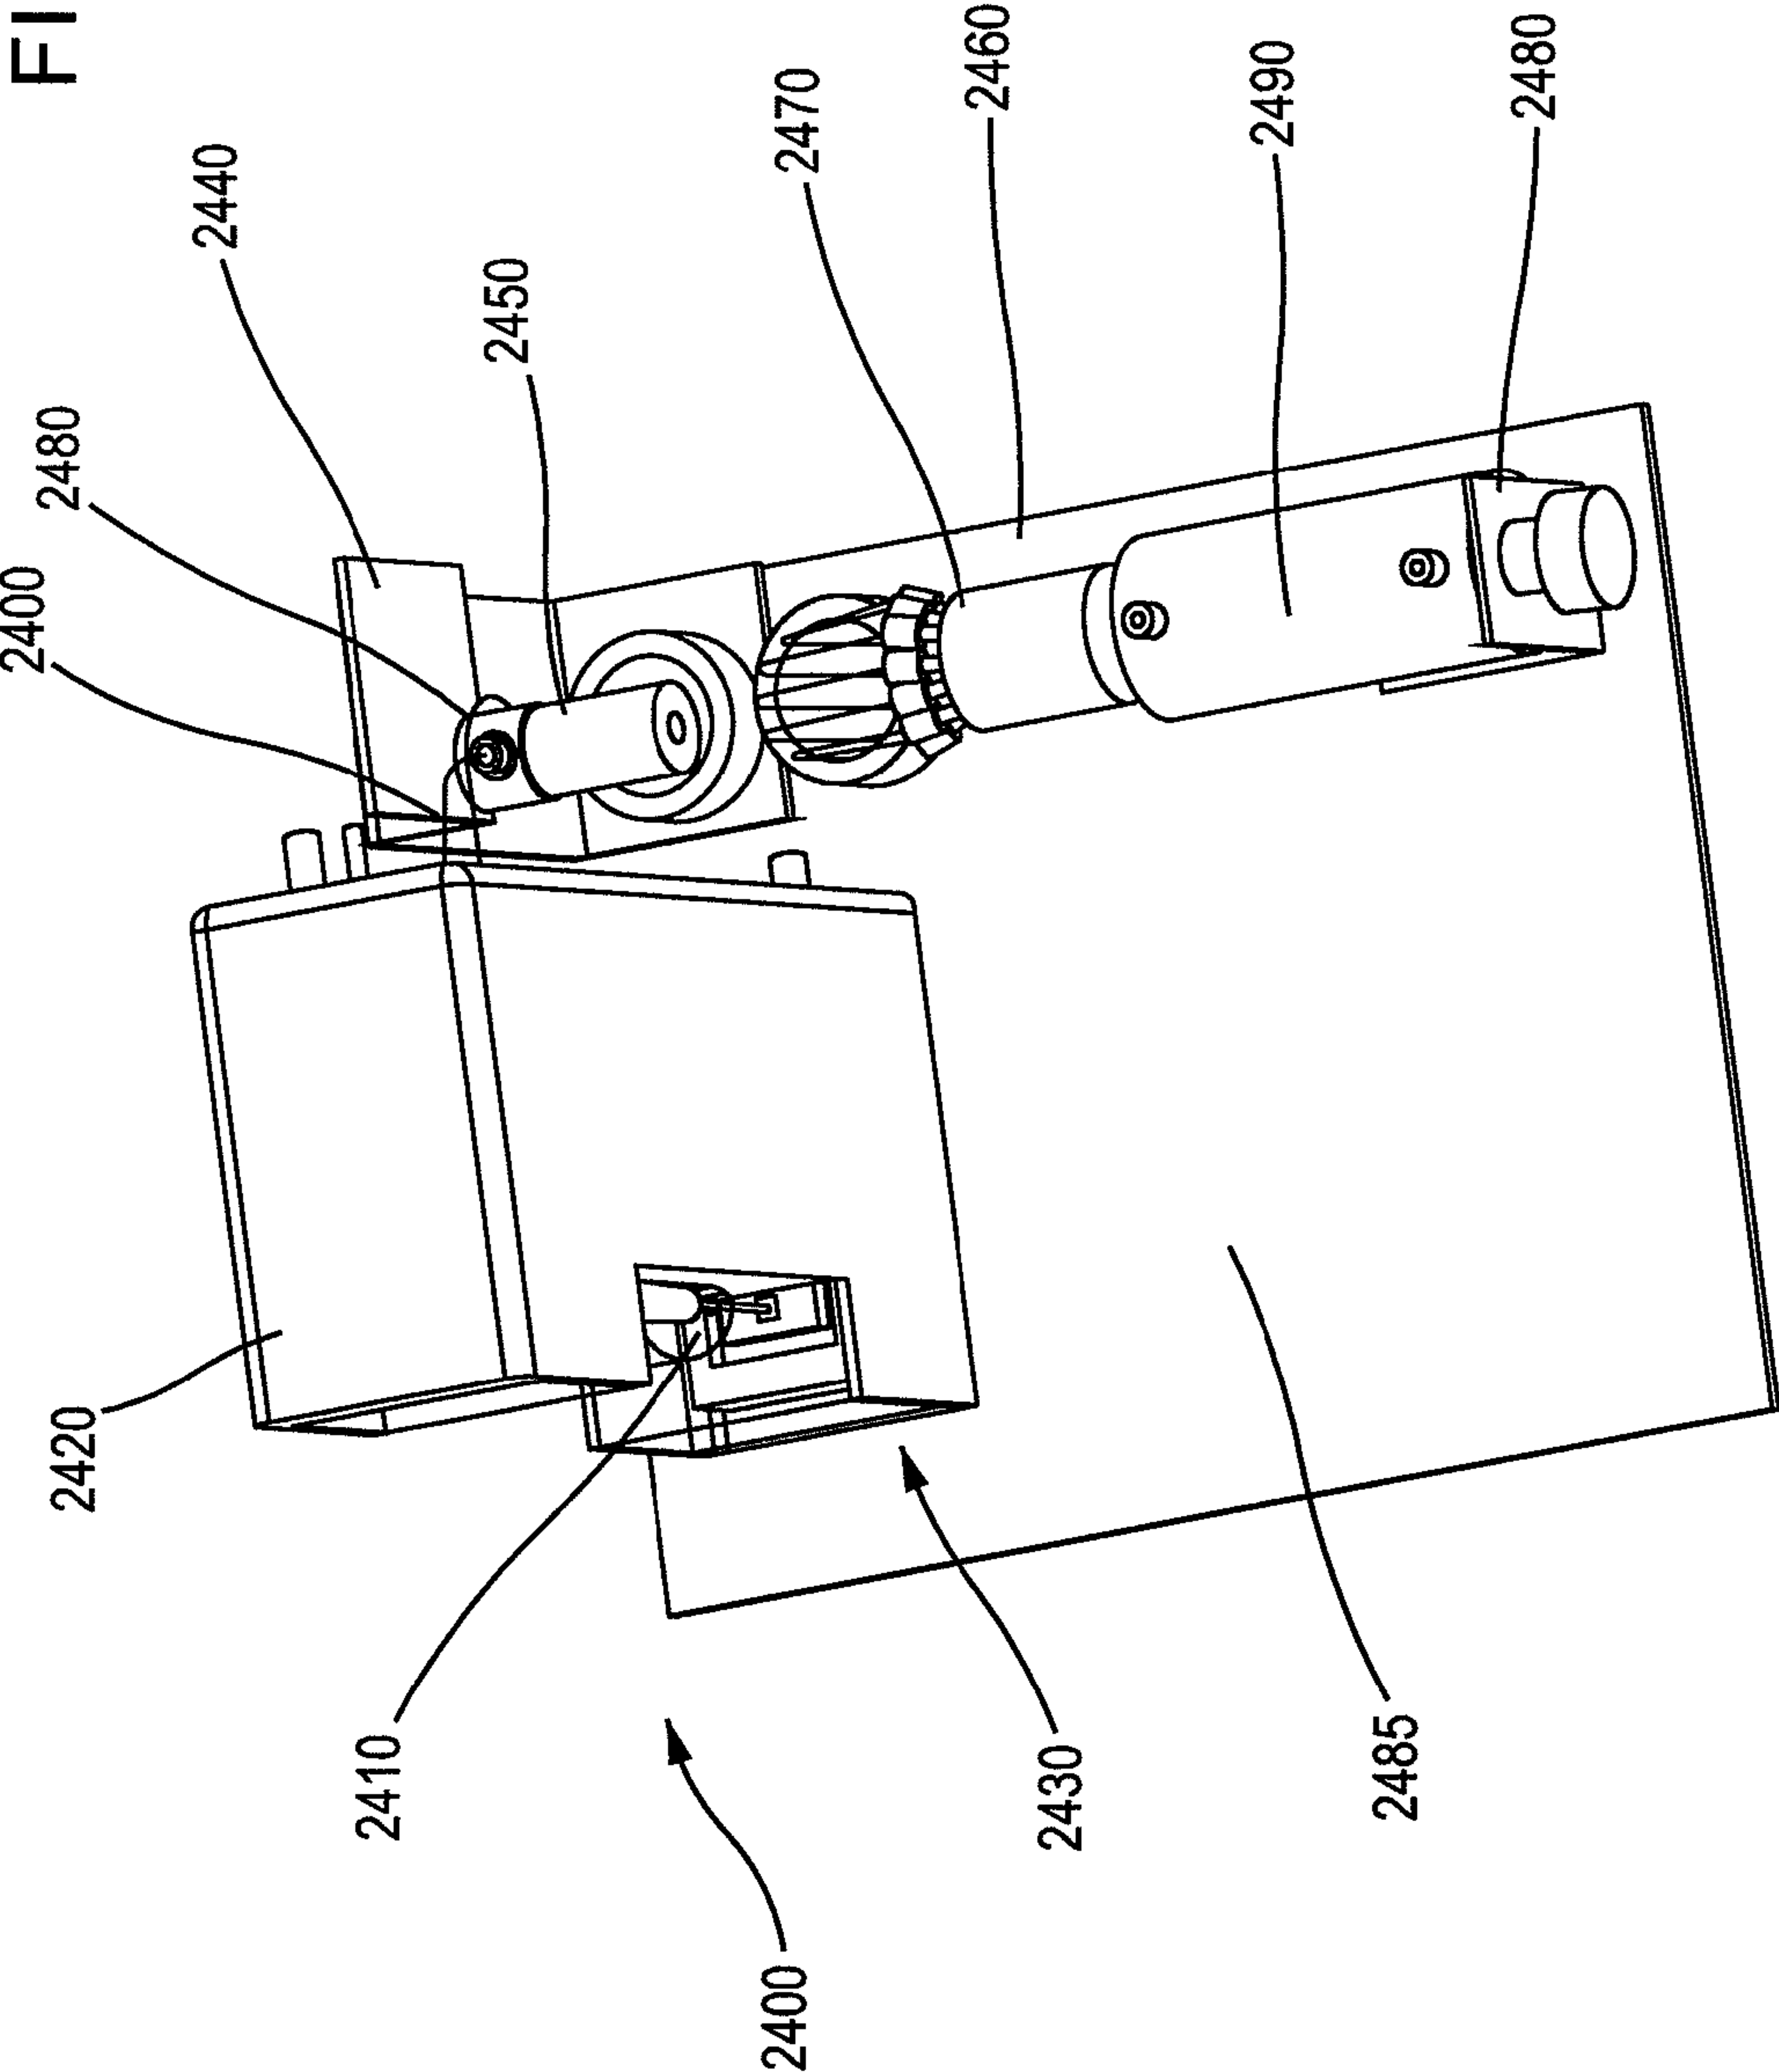

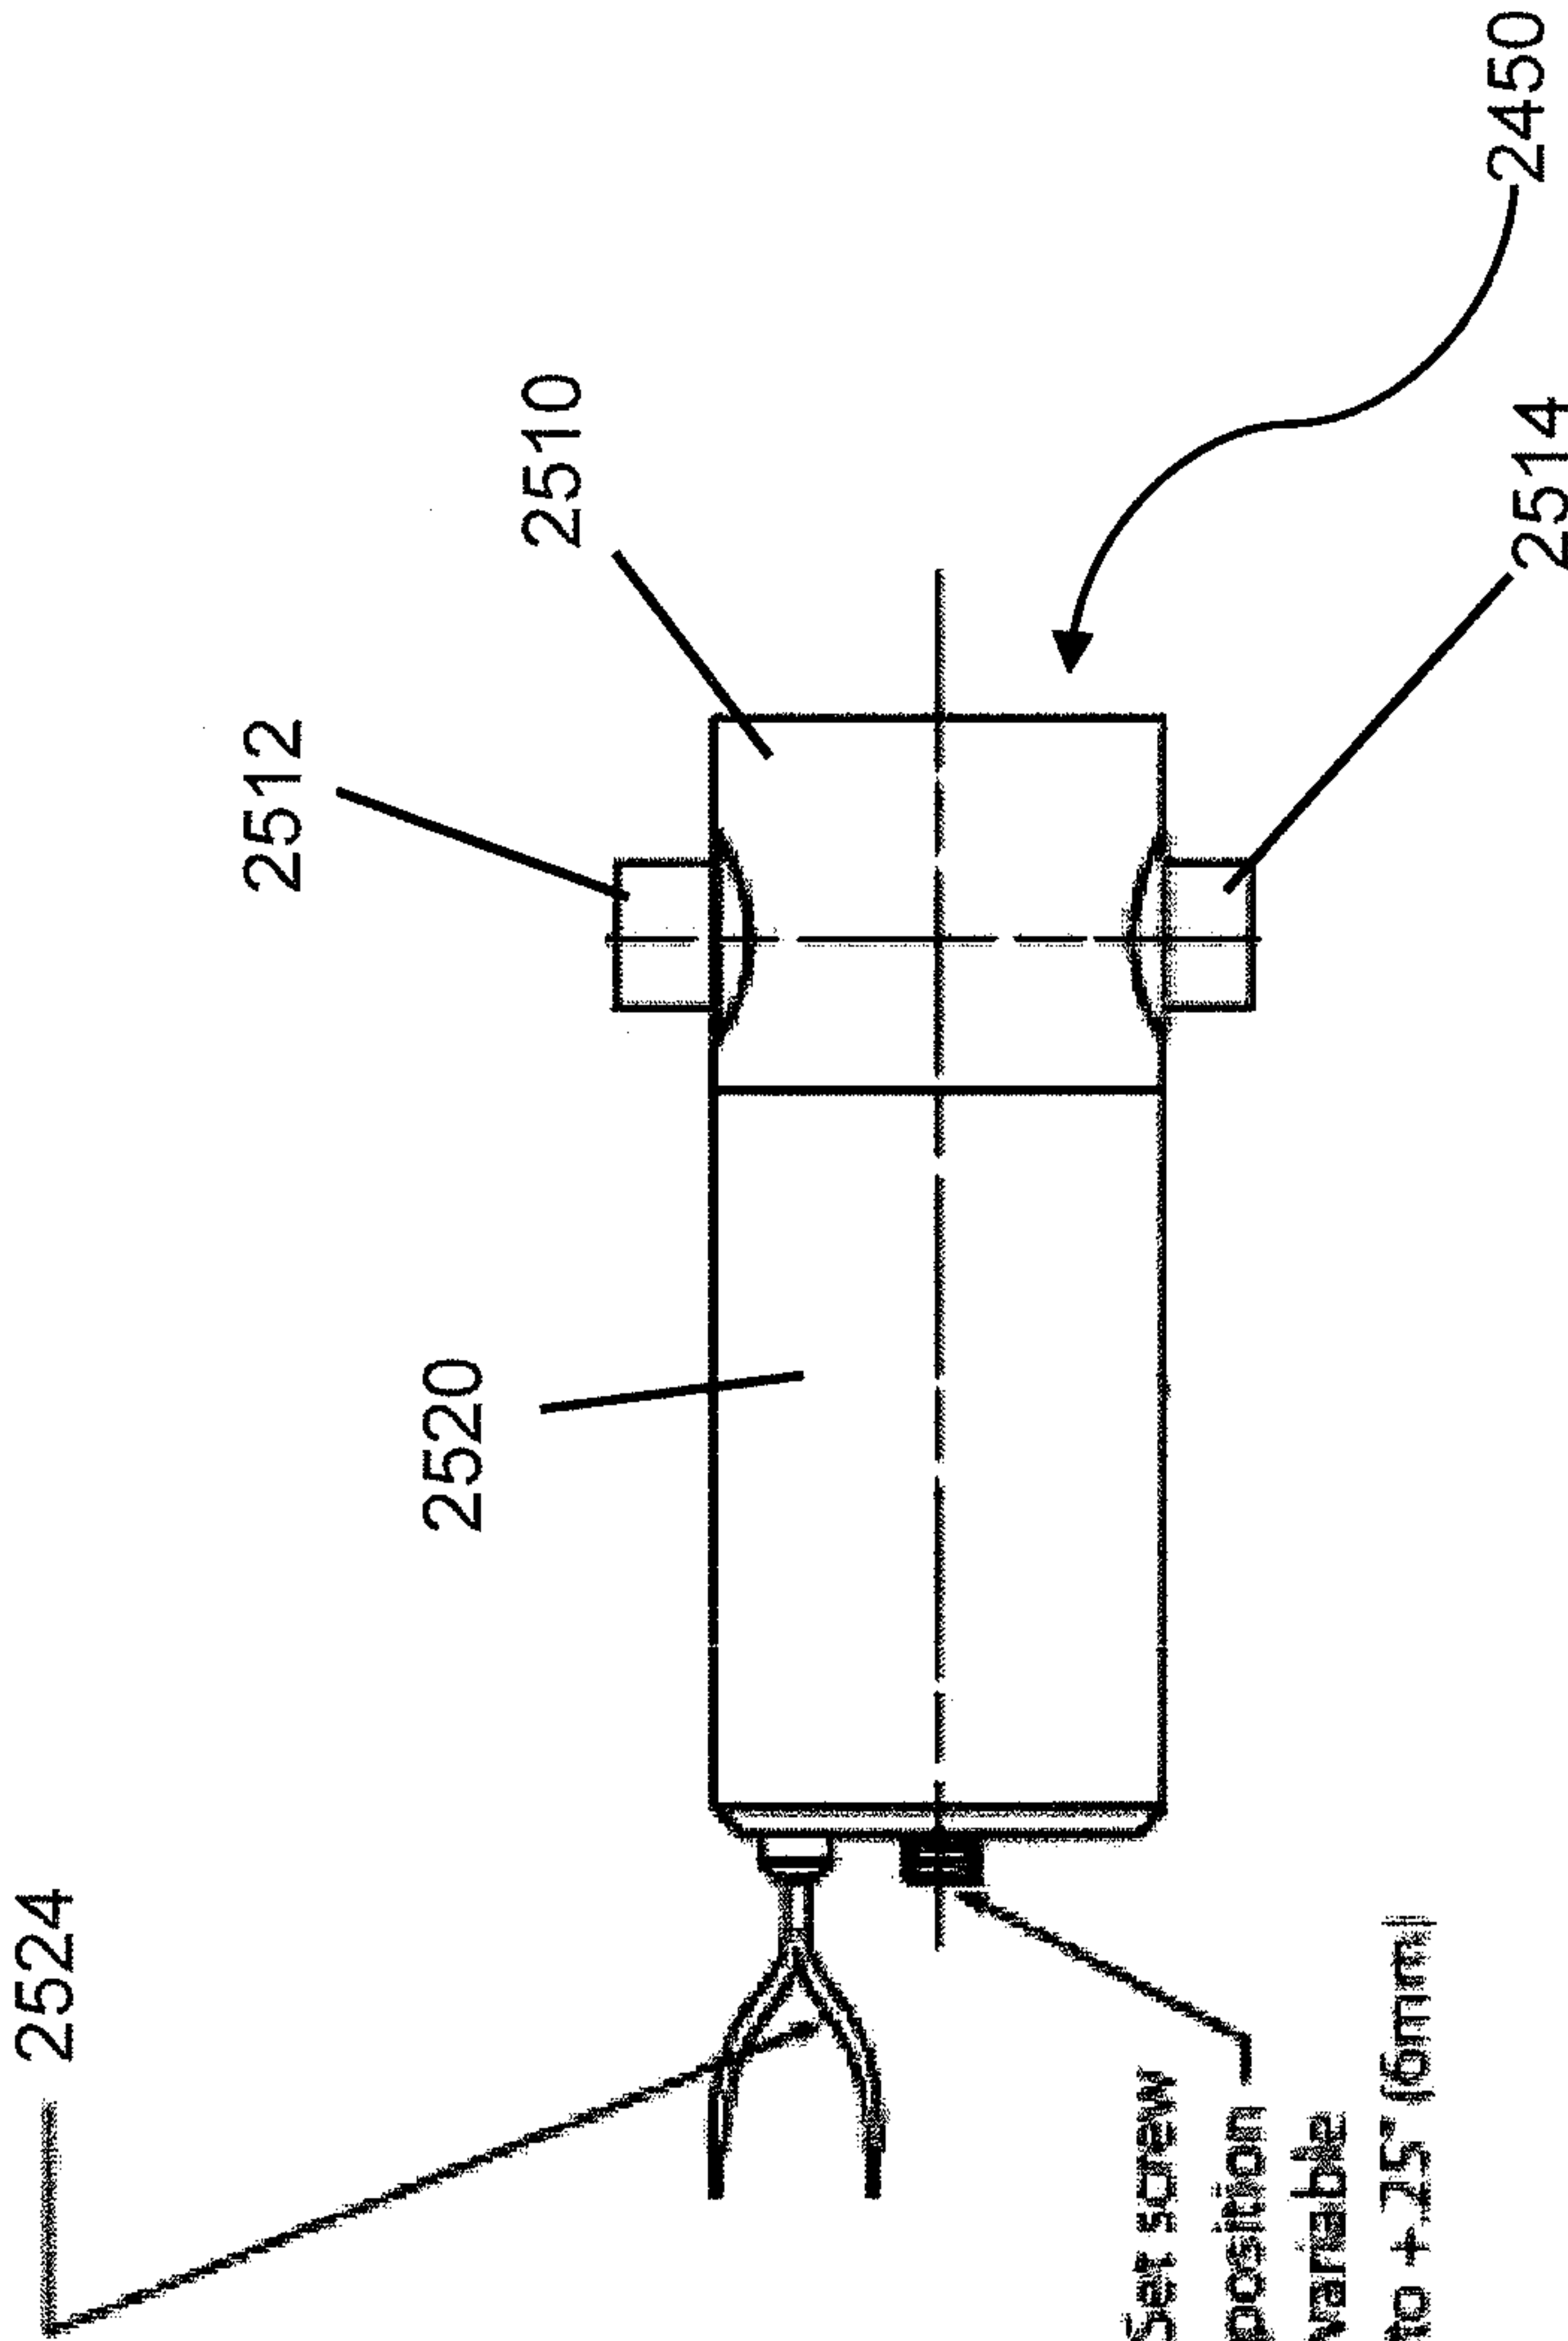


FIG. 25A

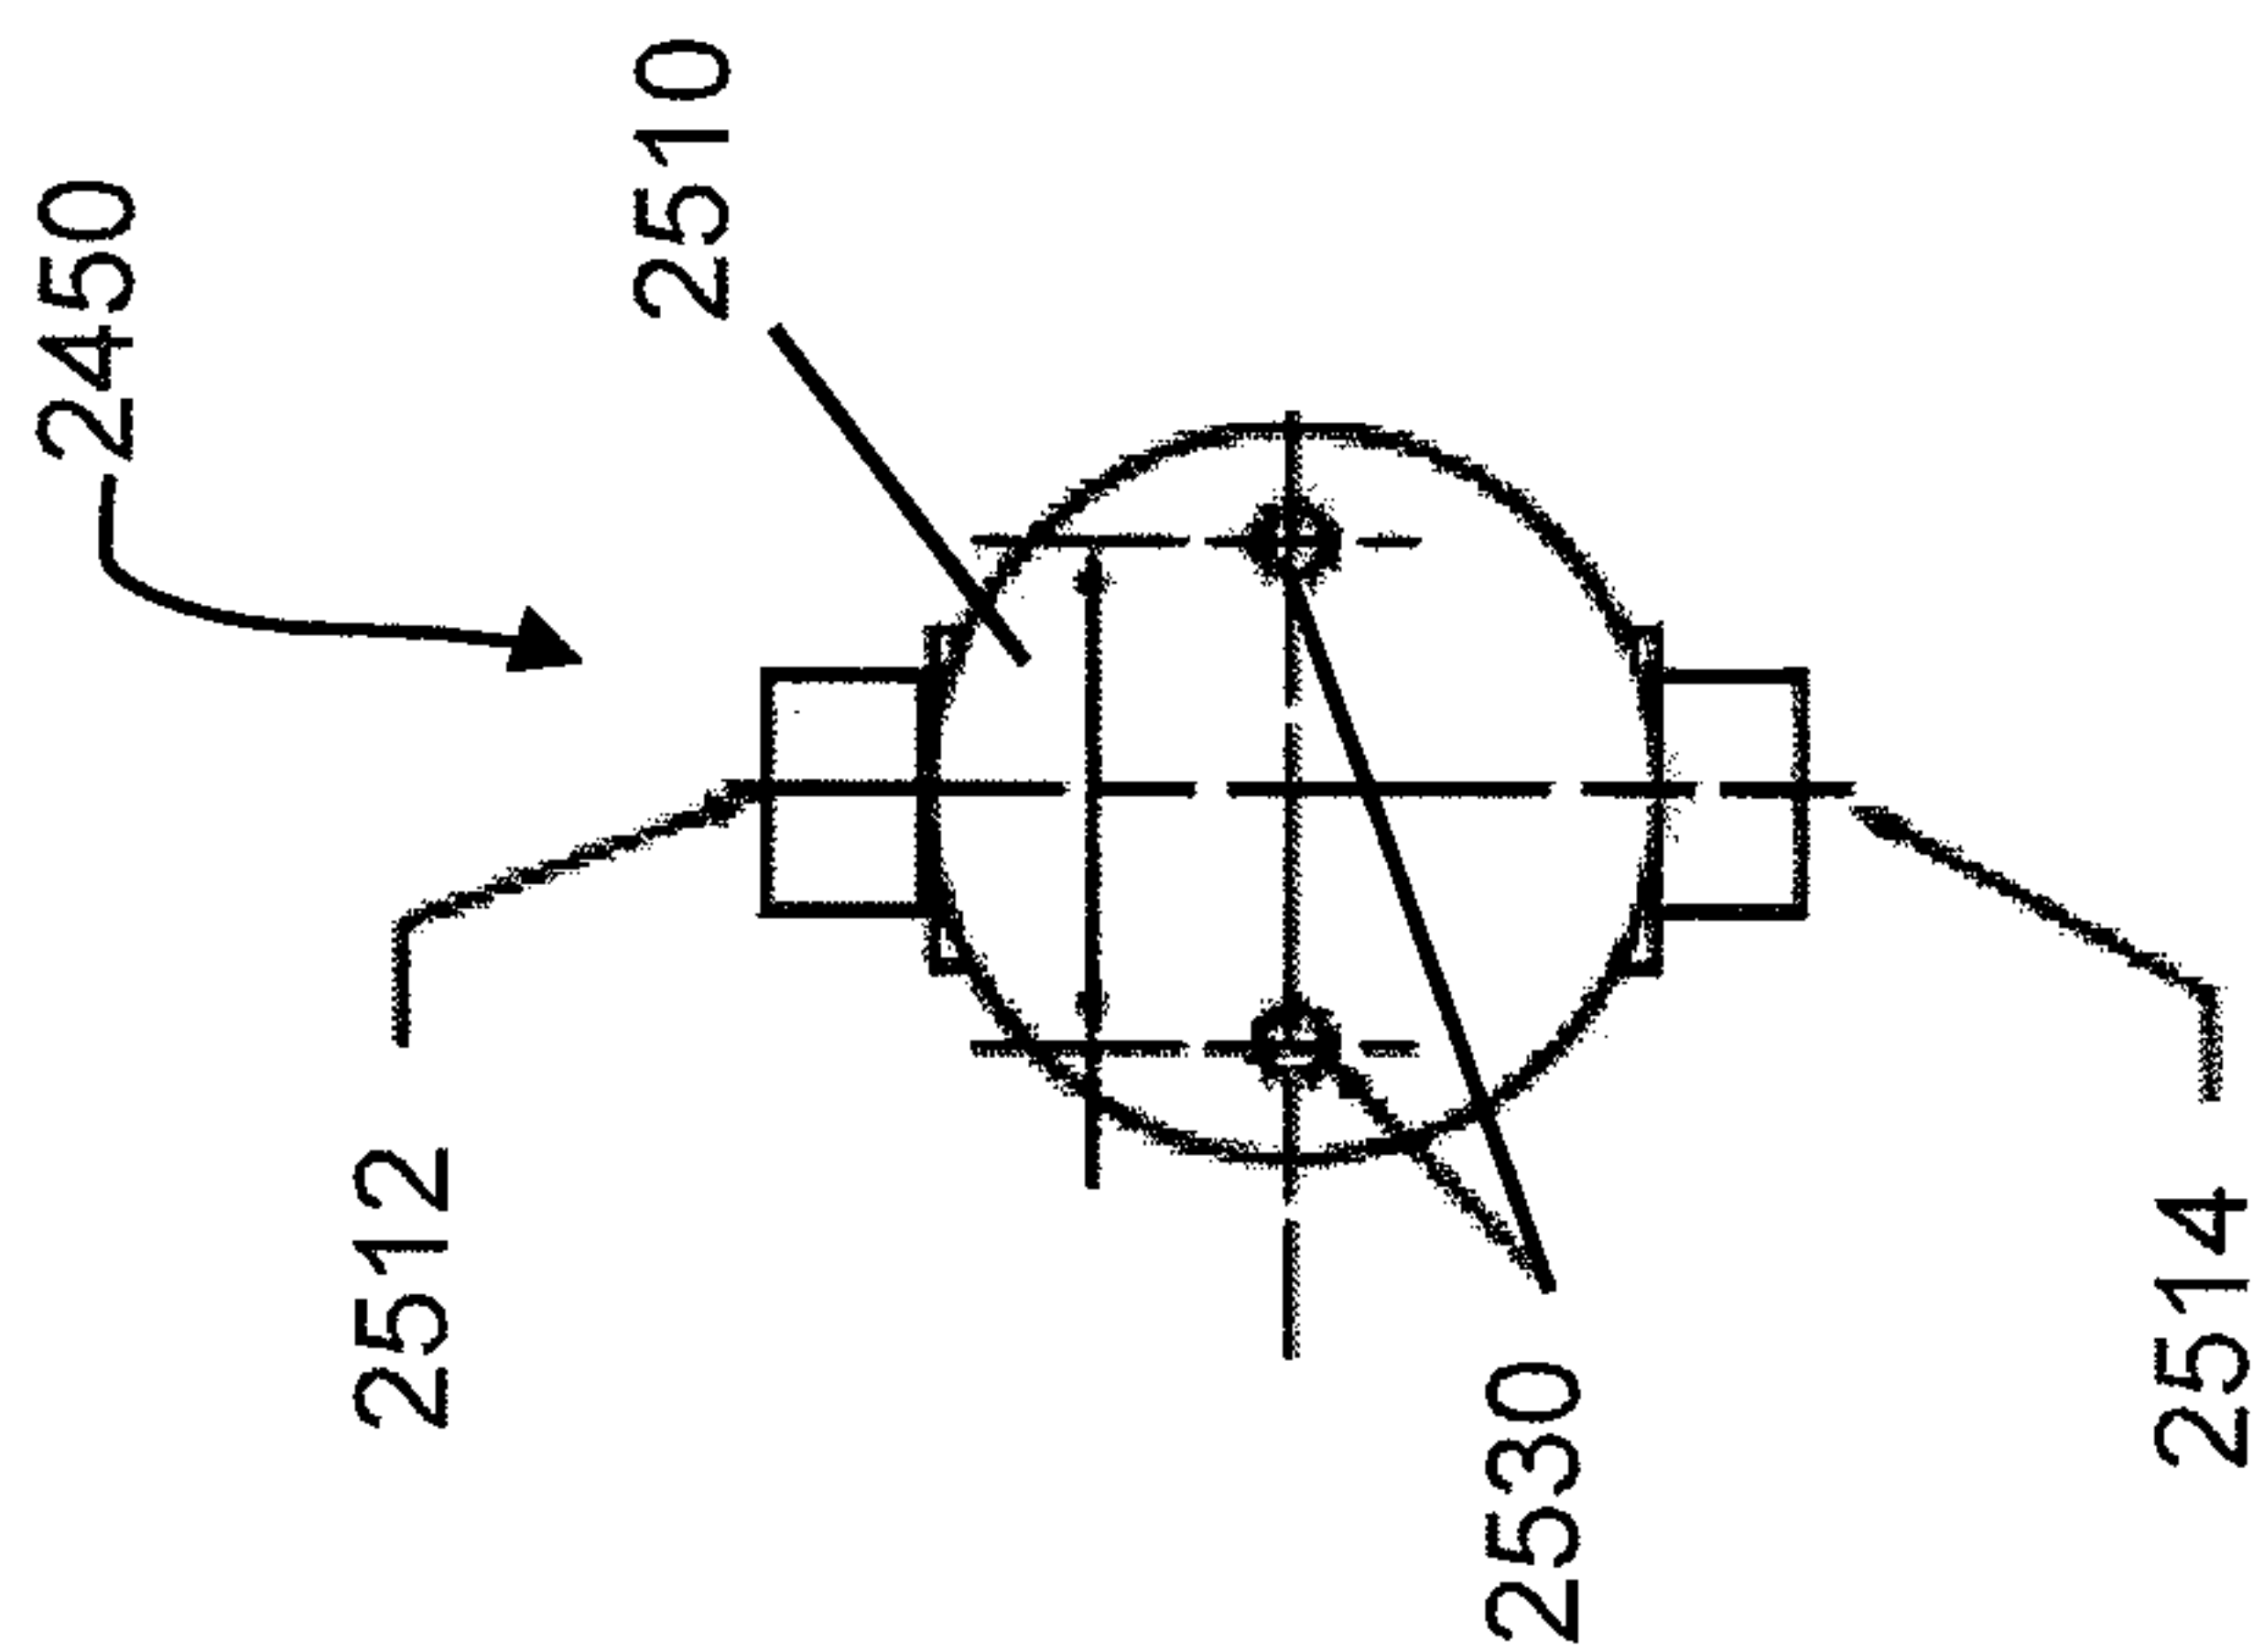


FIG. 25B




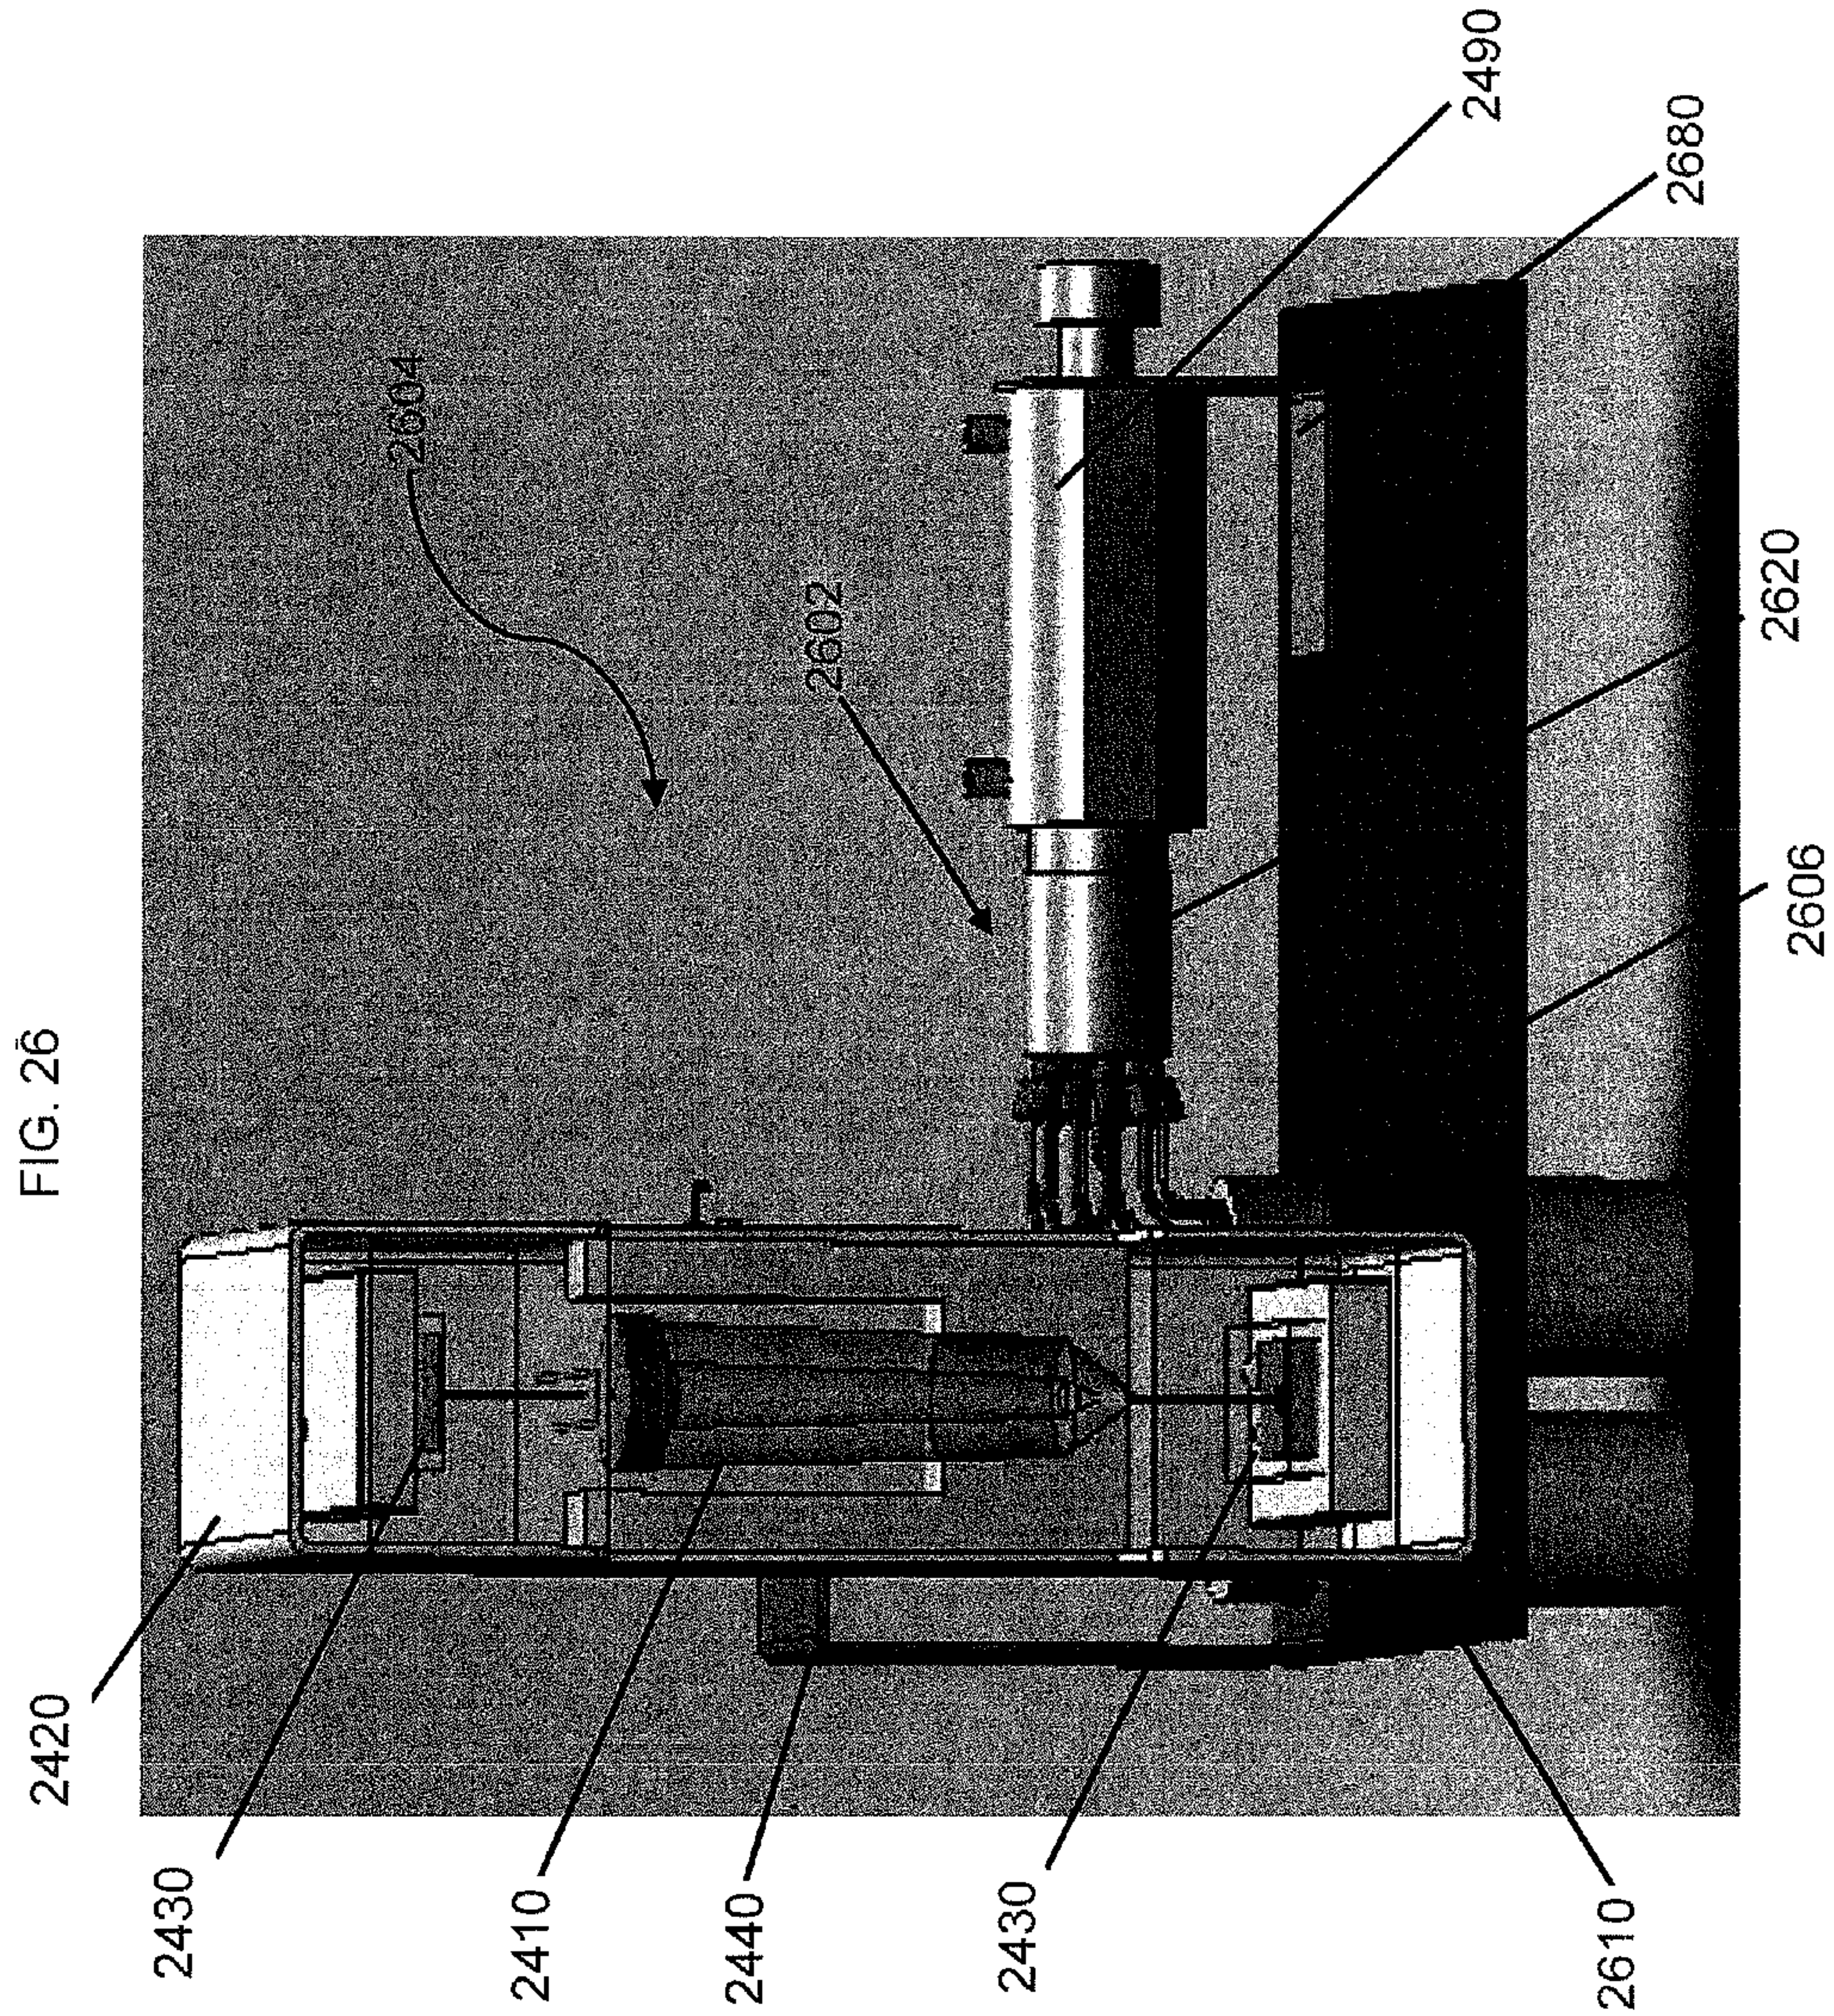




FIG. 27

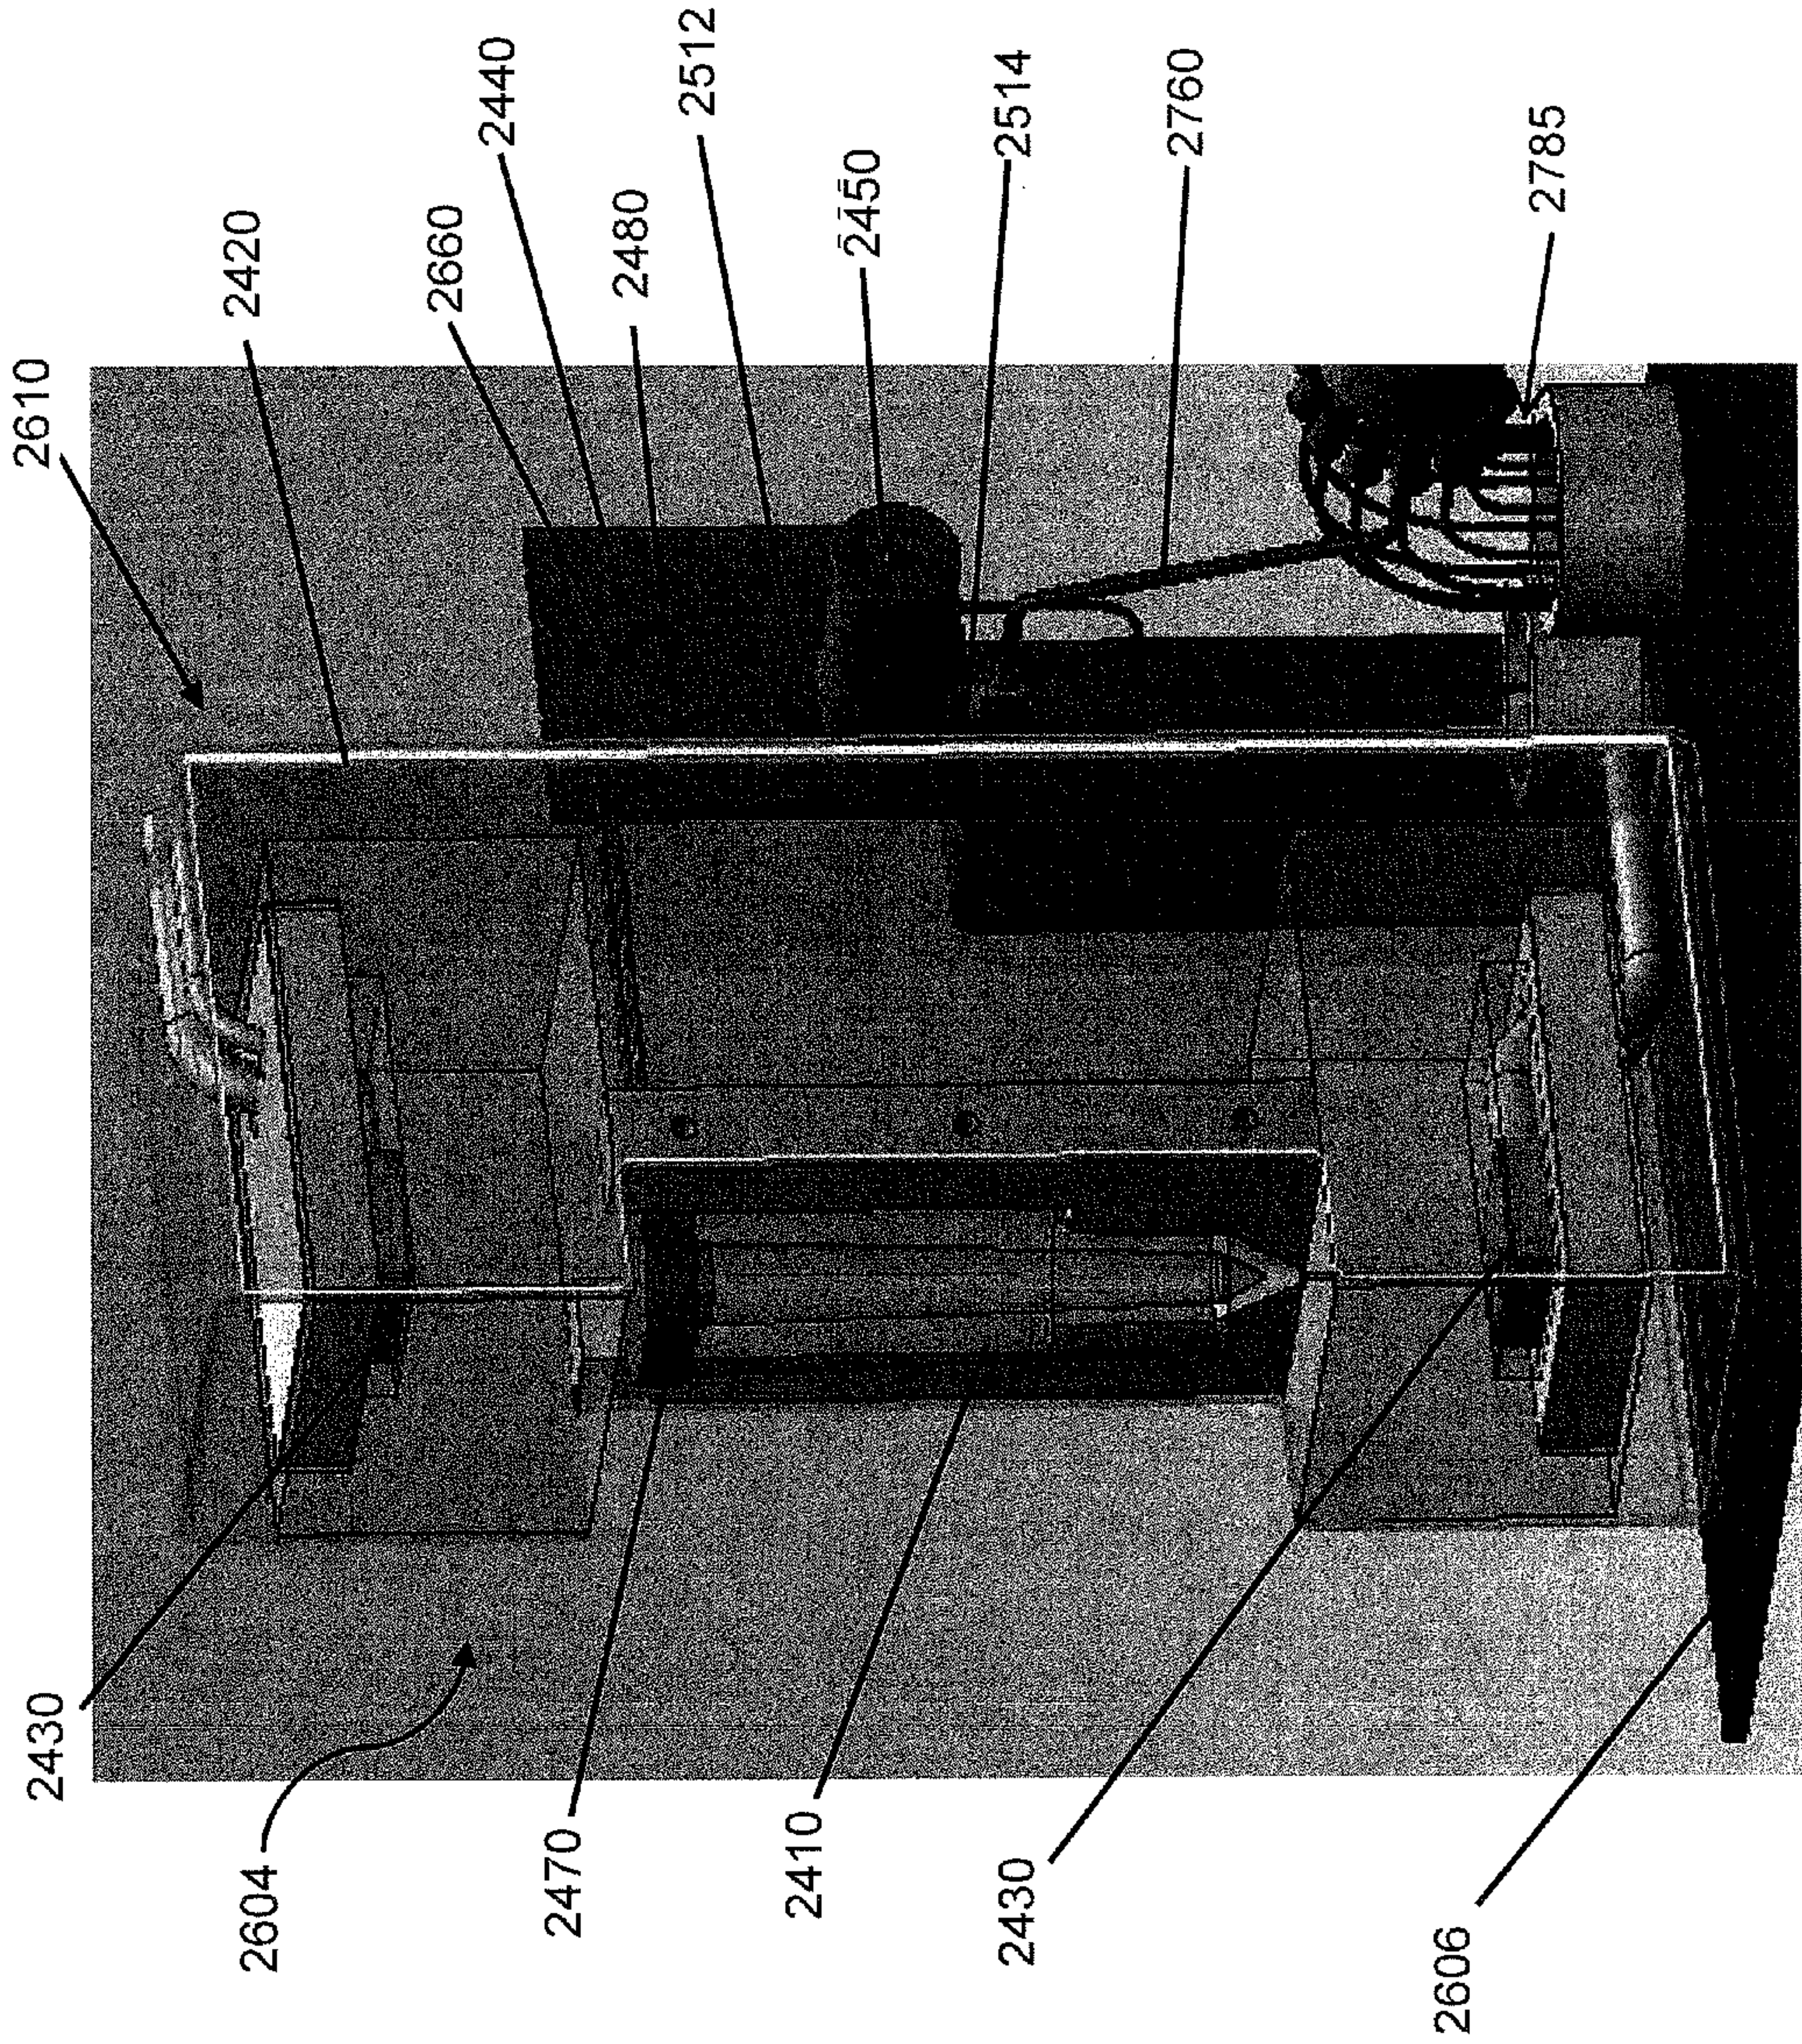





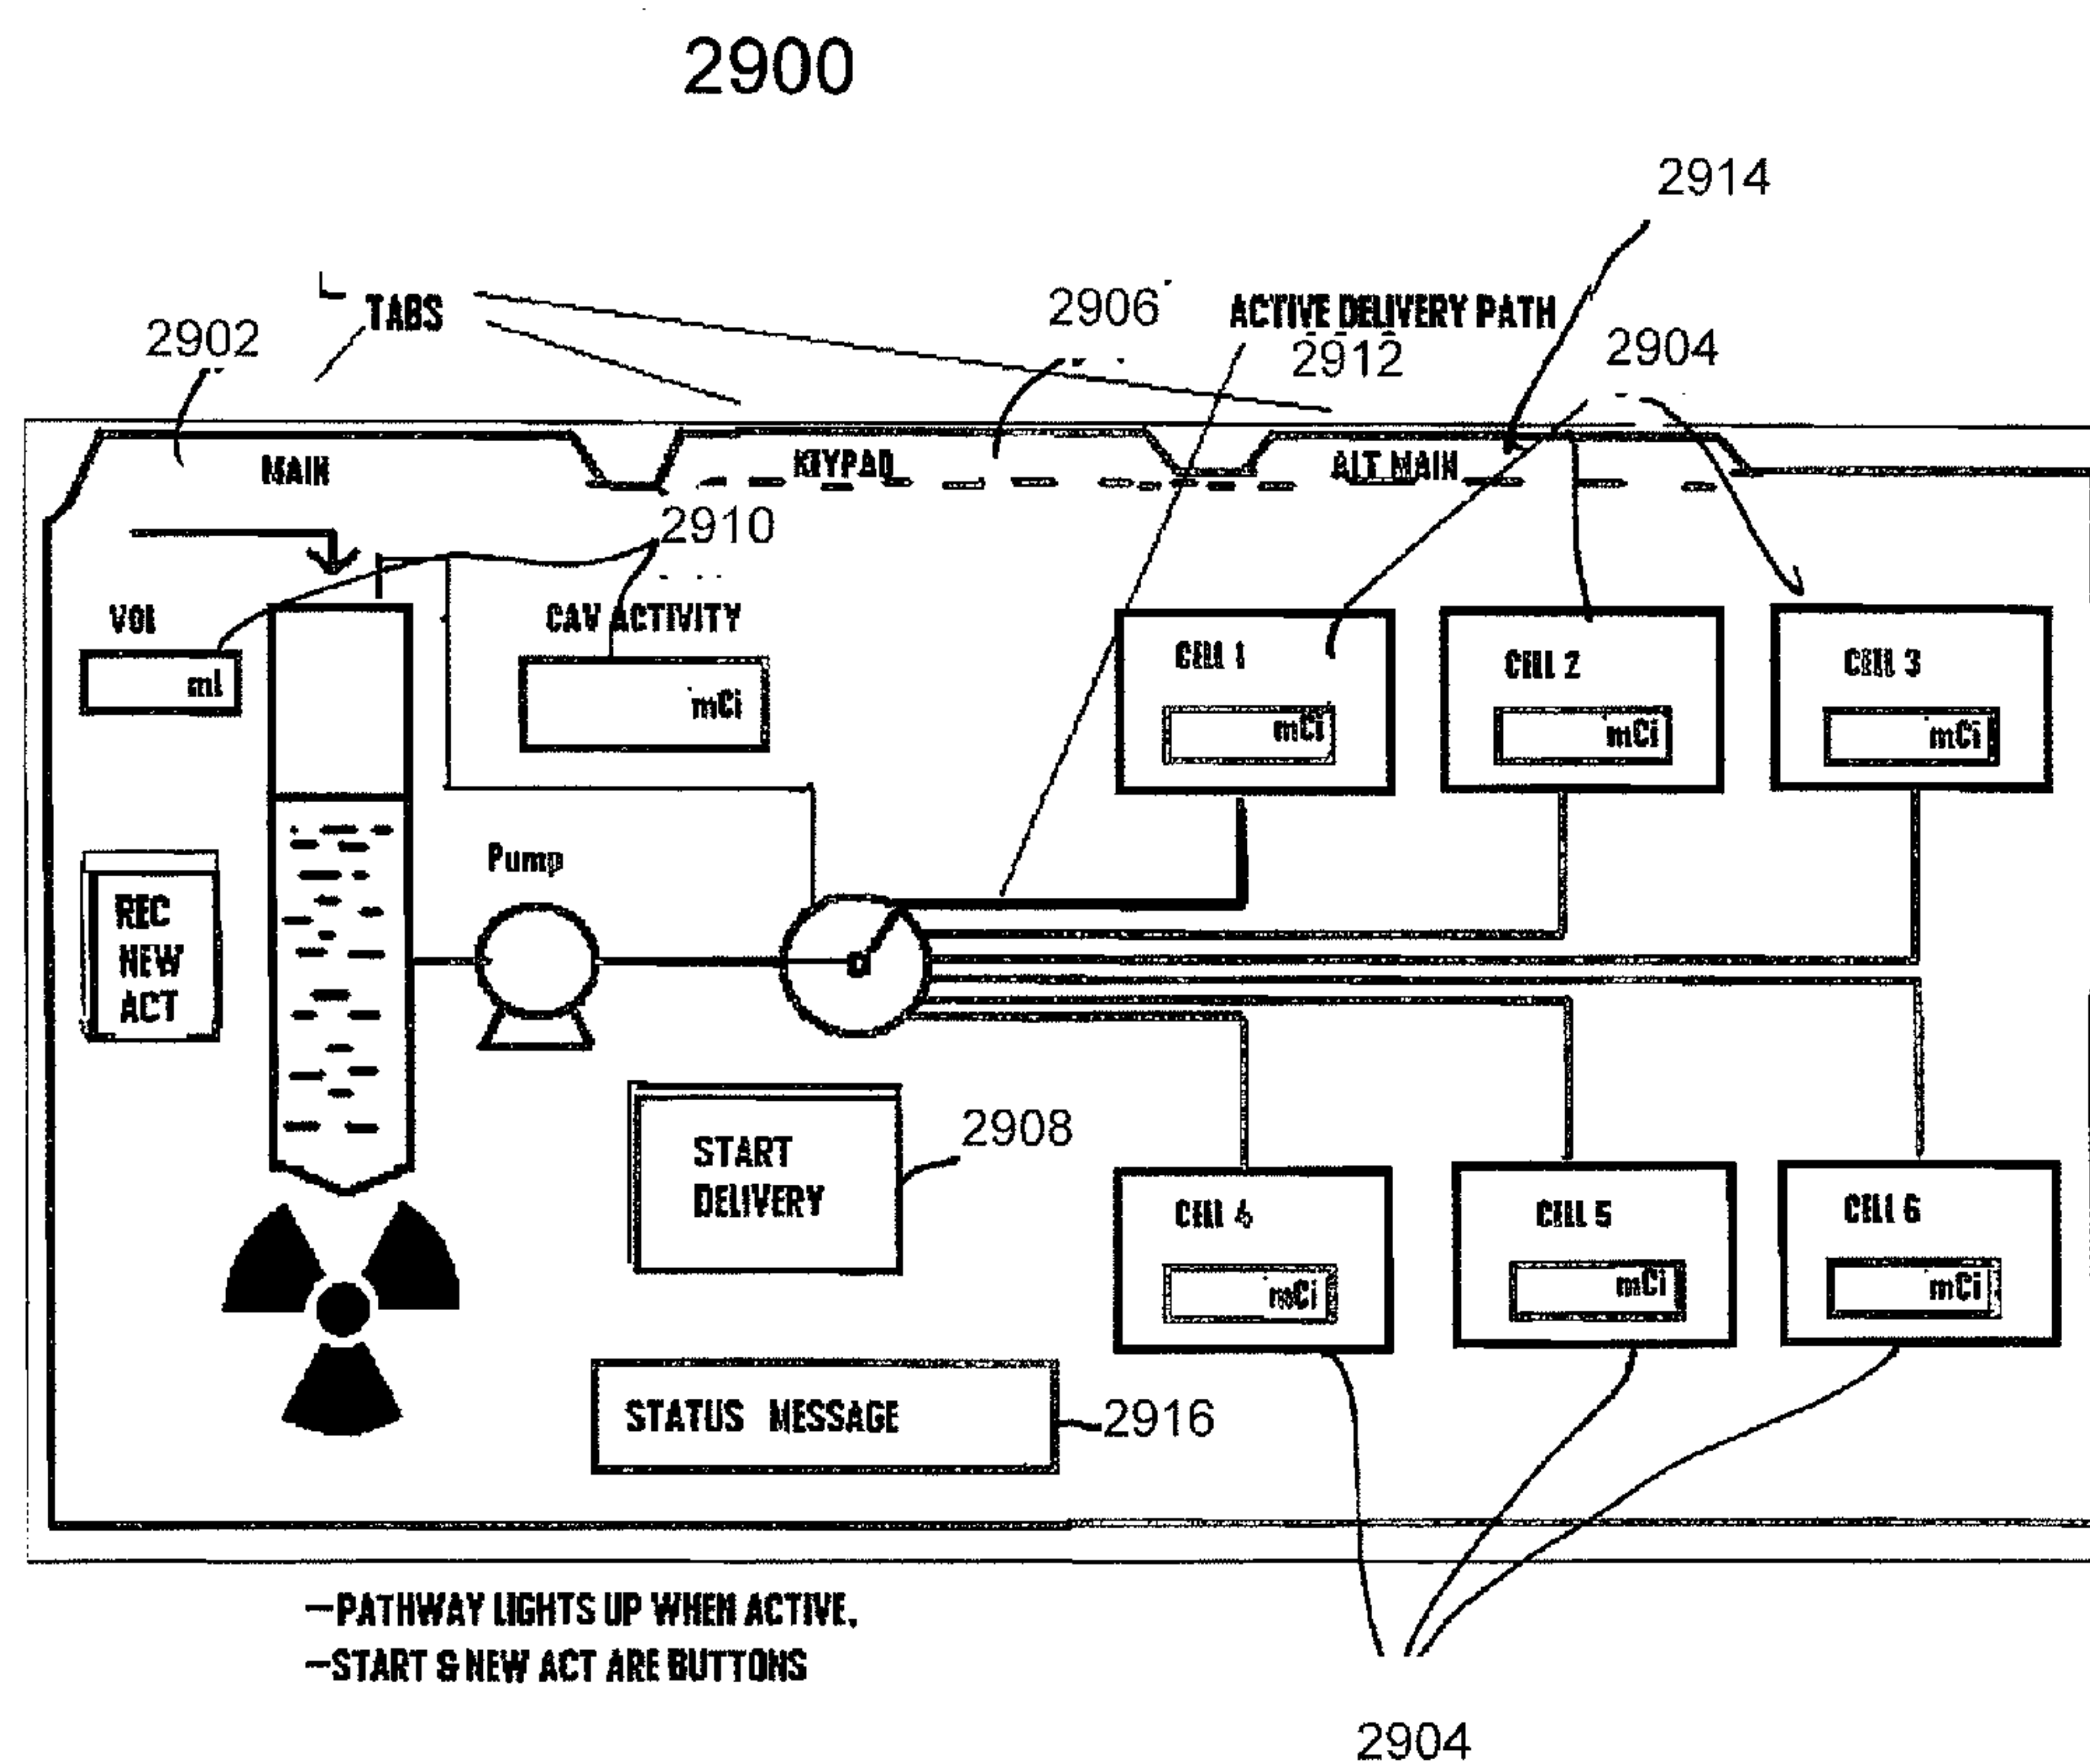


FIG. 29



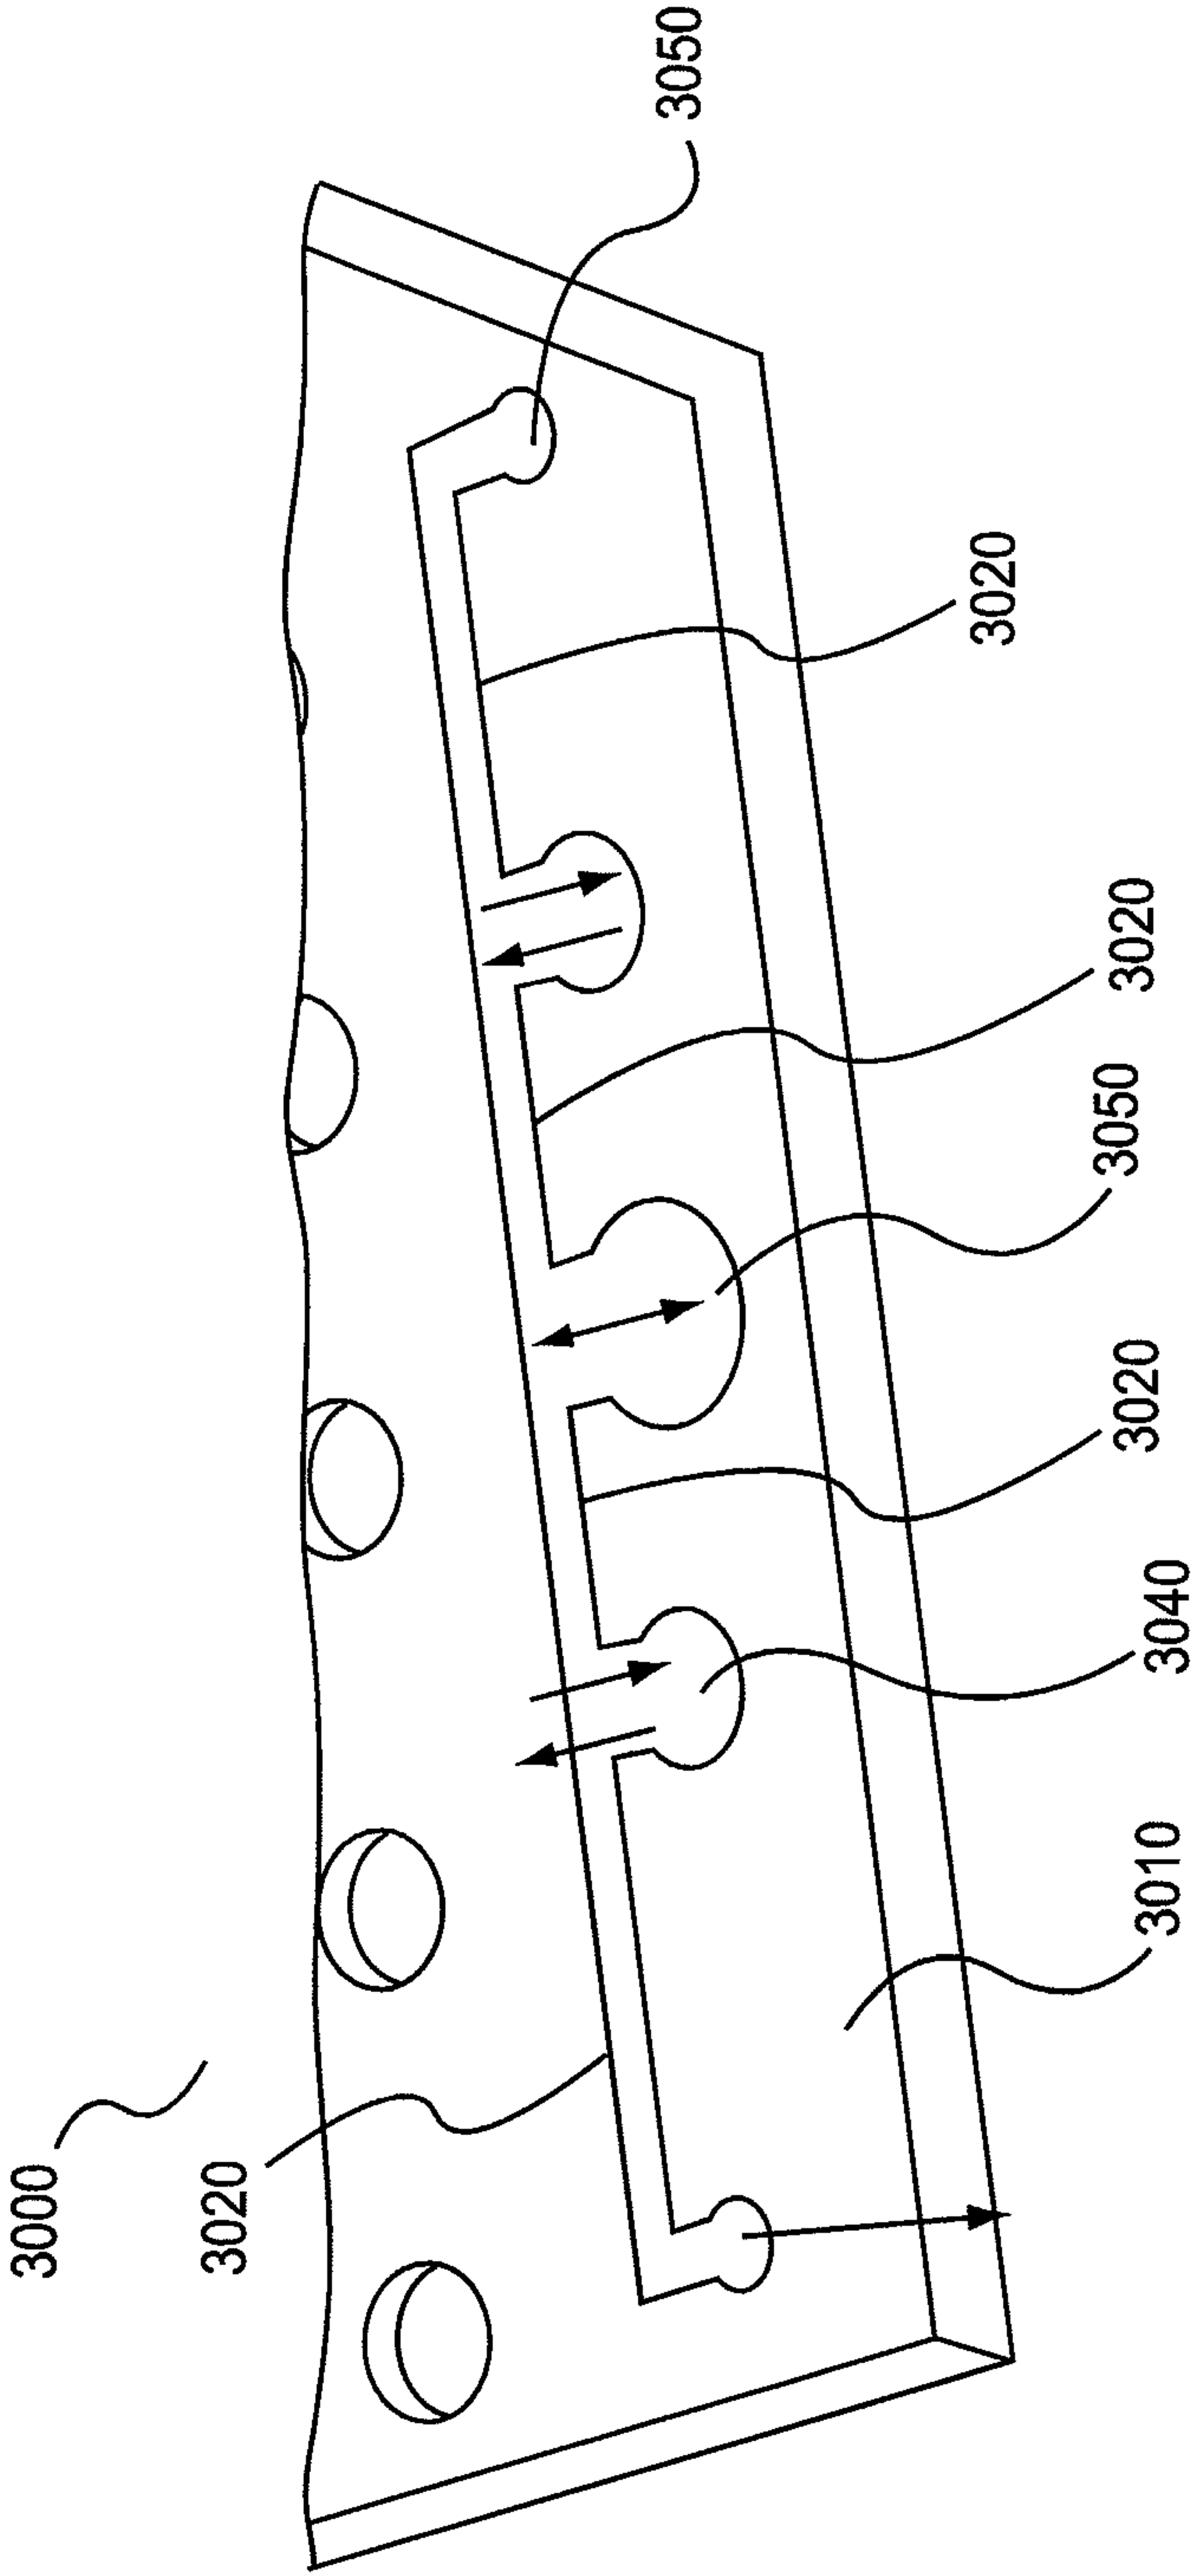


FIG. 30

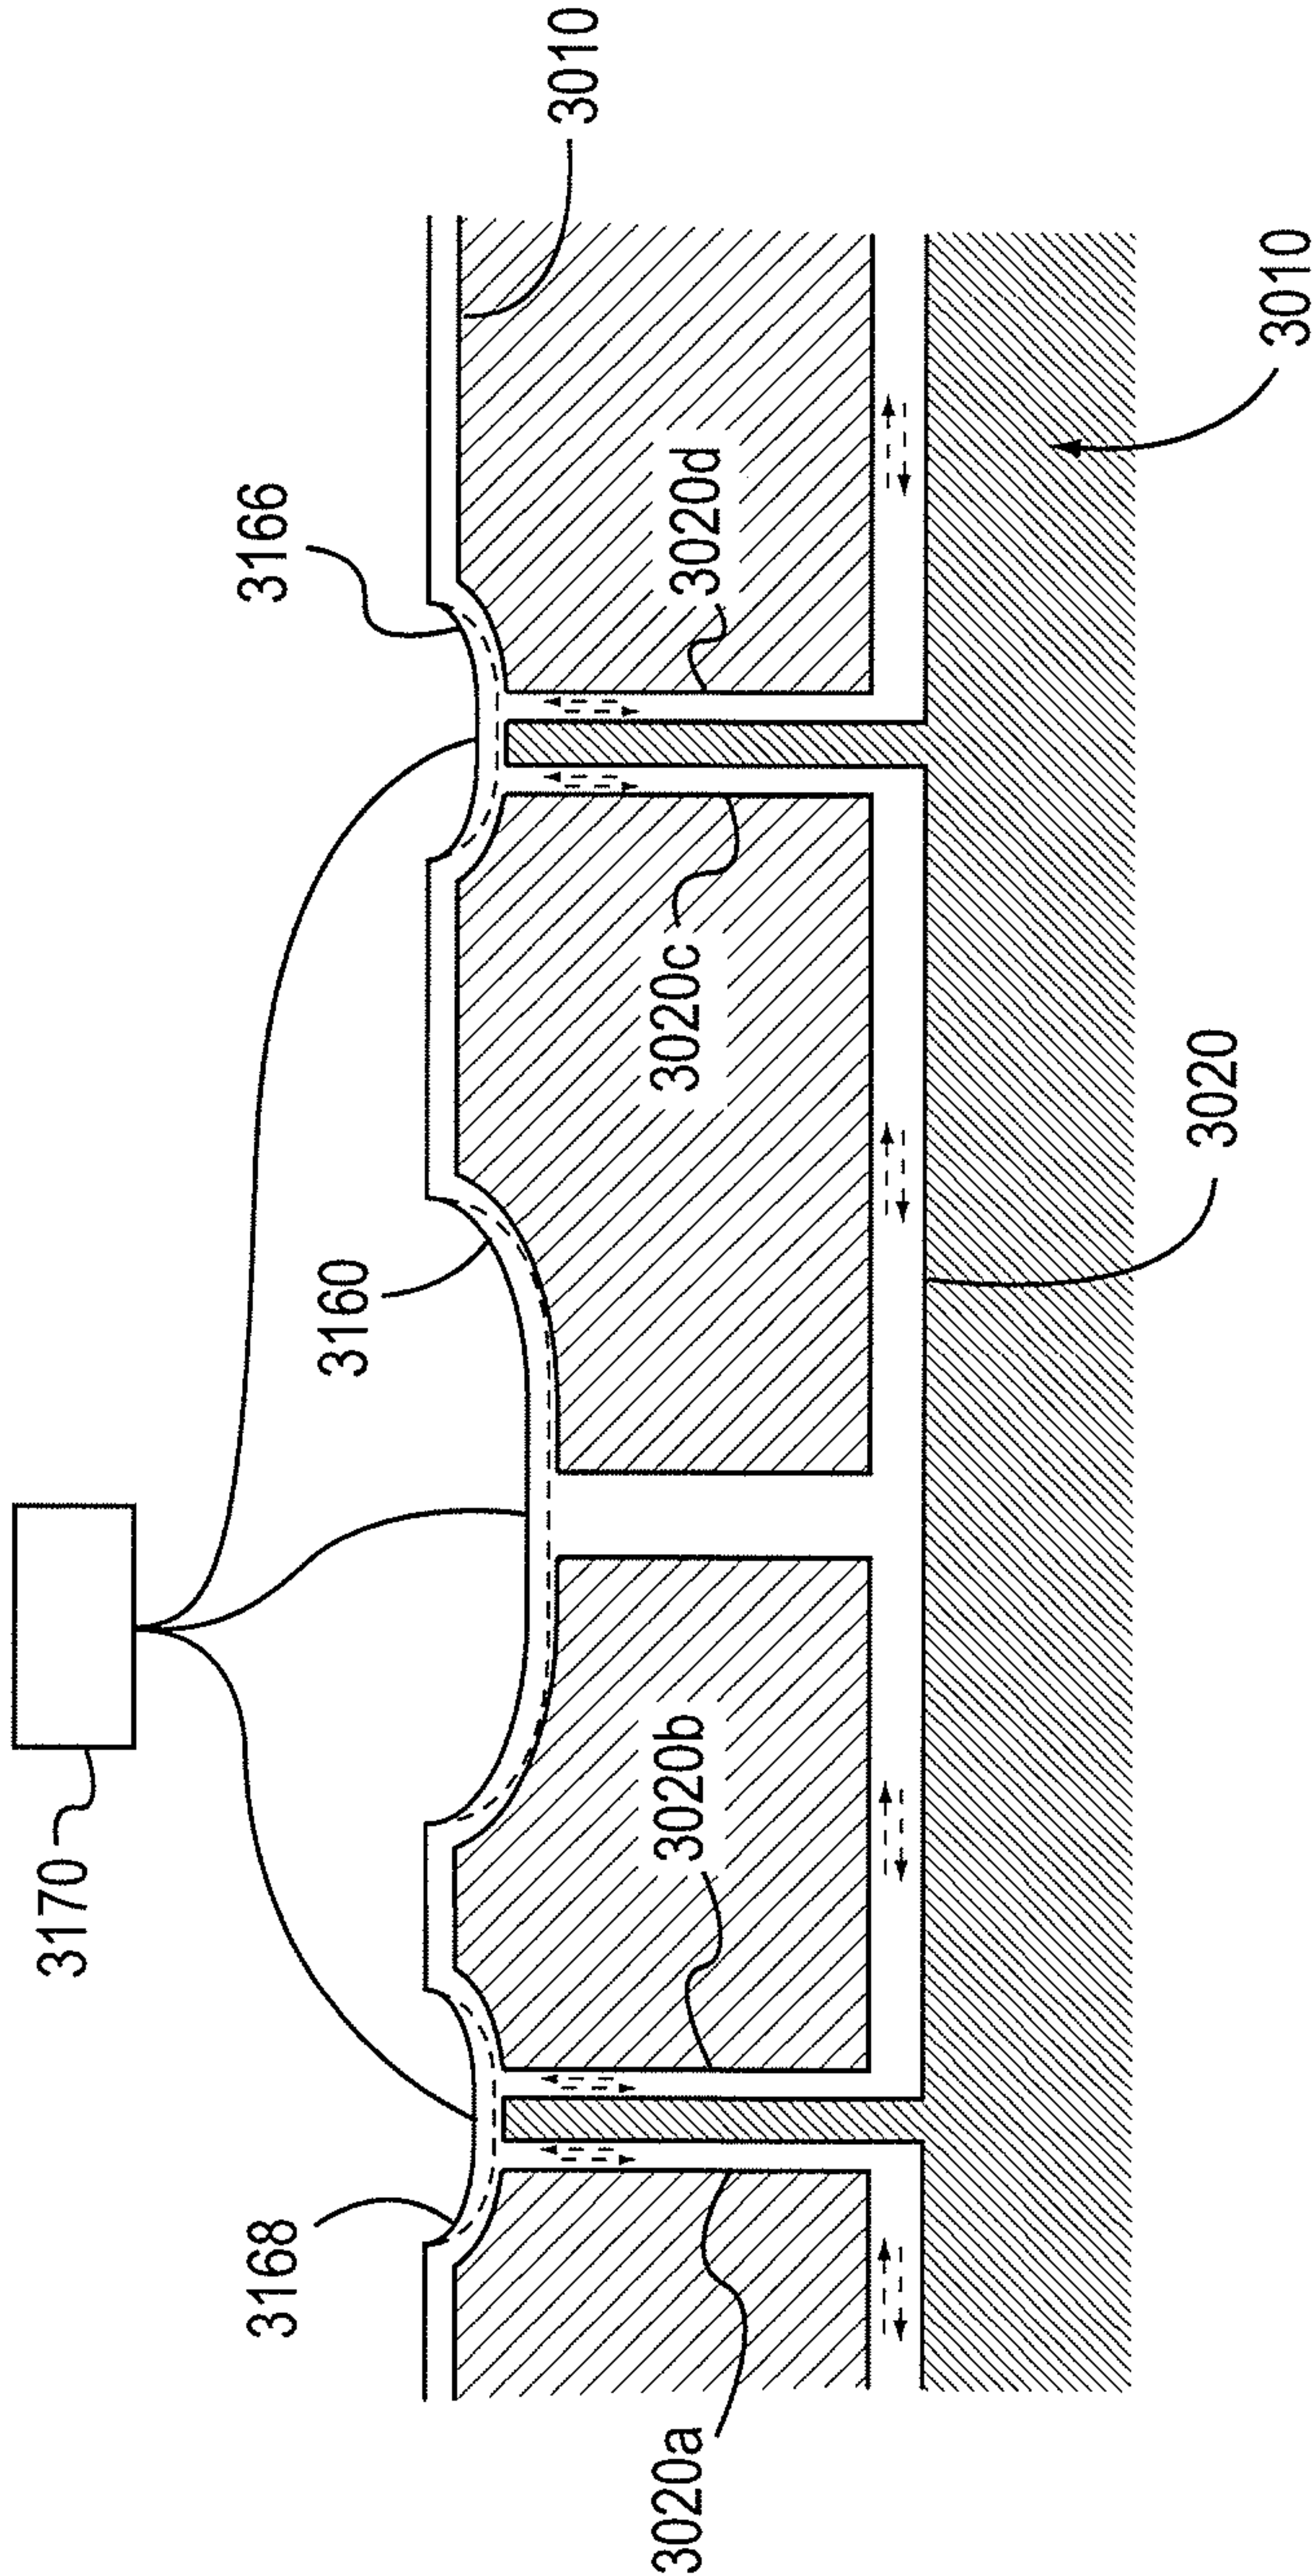


FIG.31



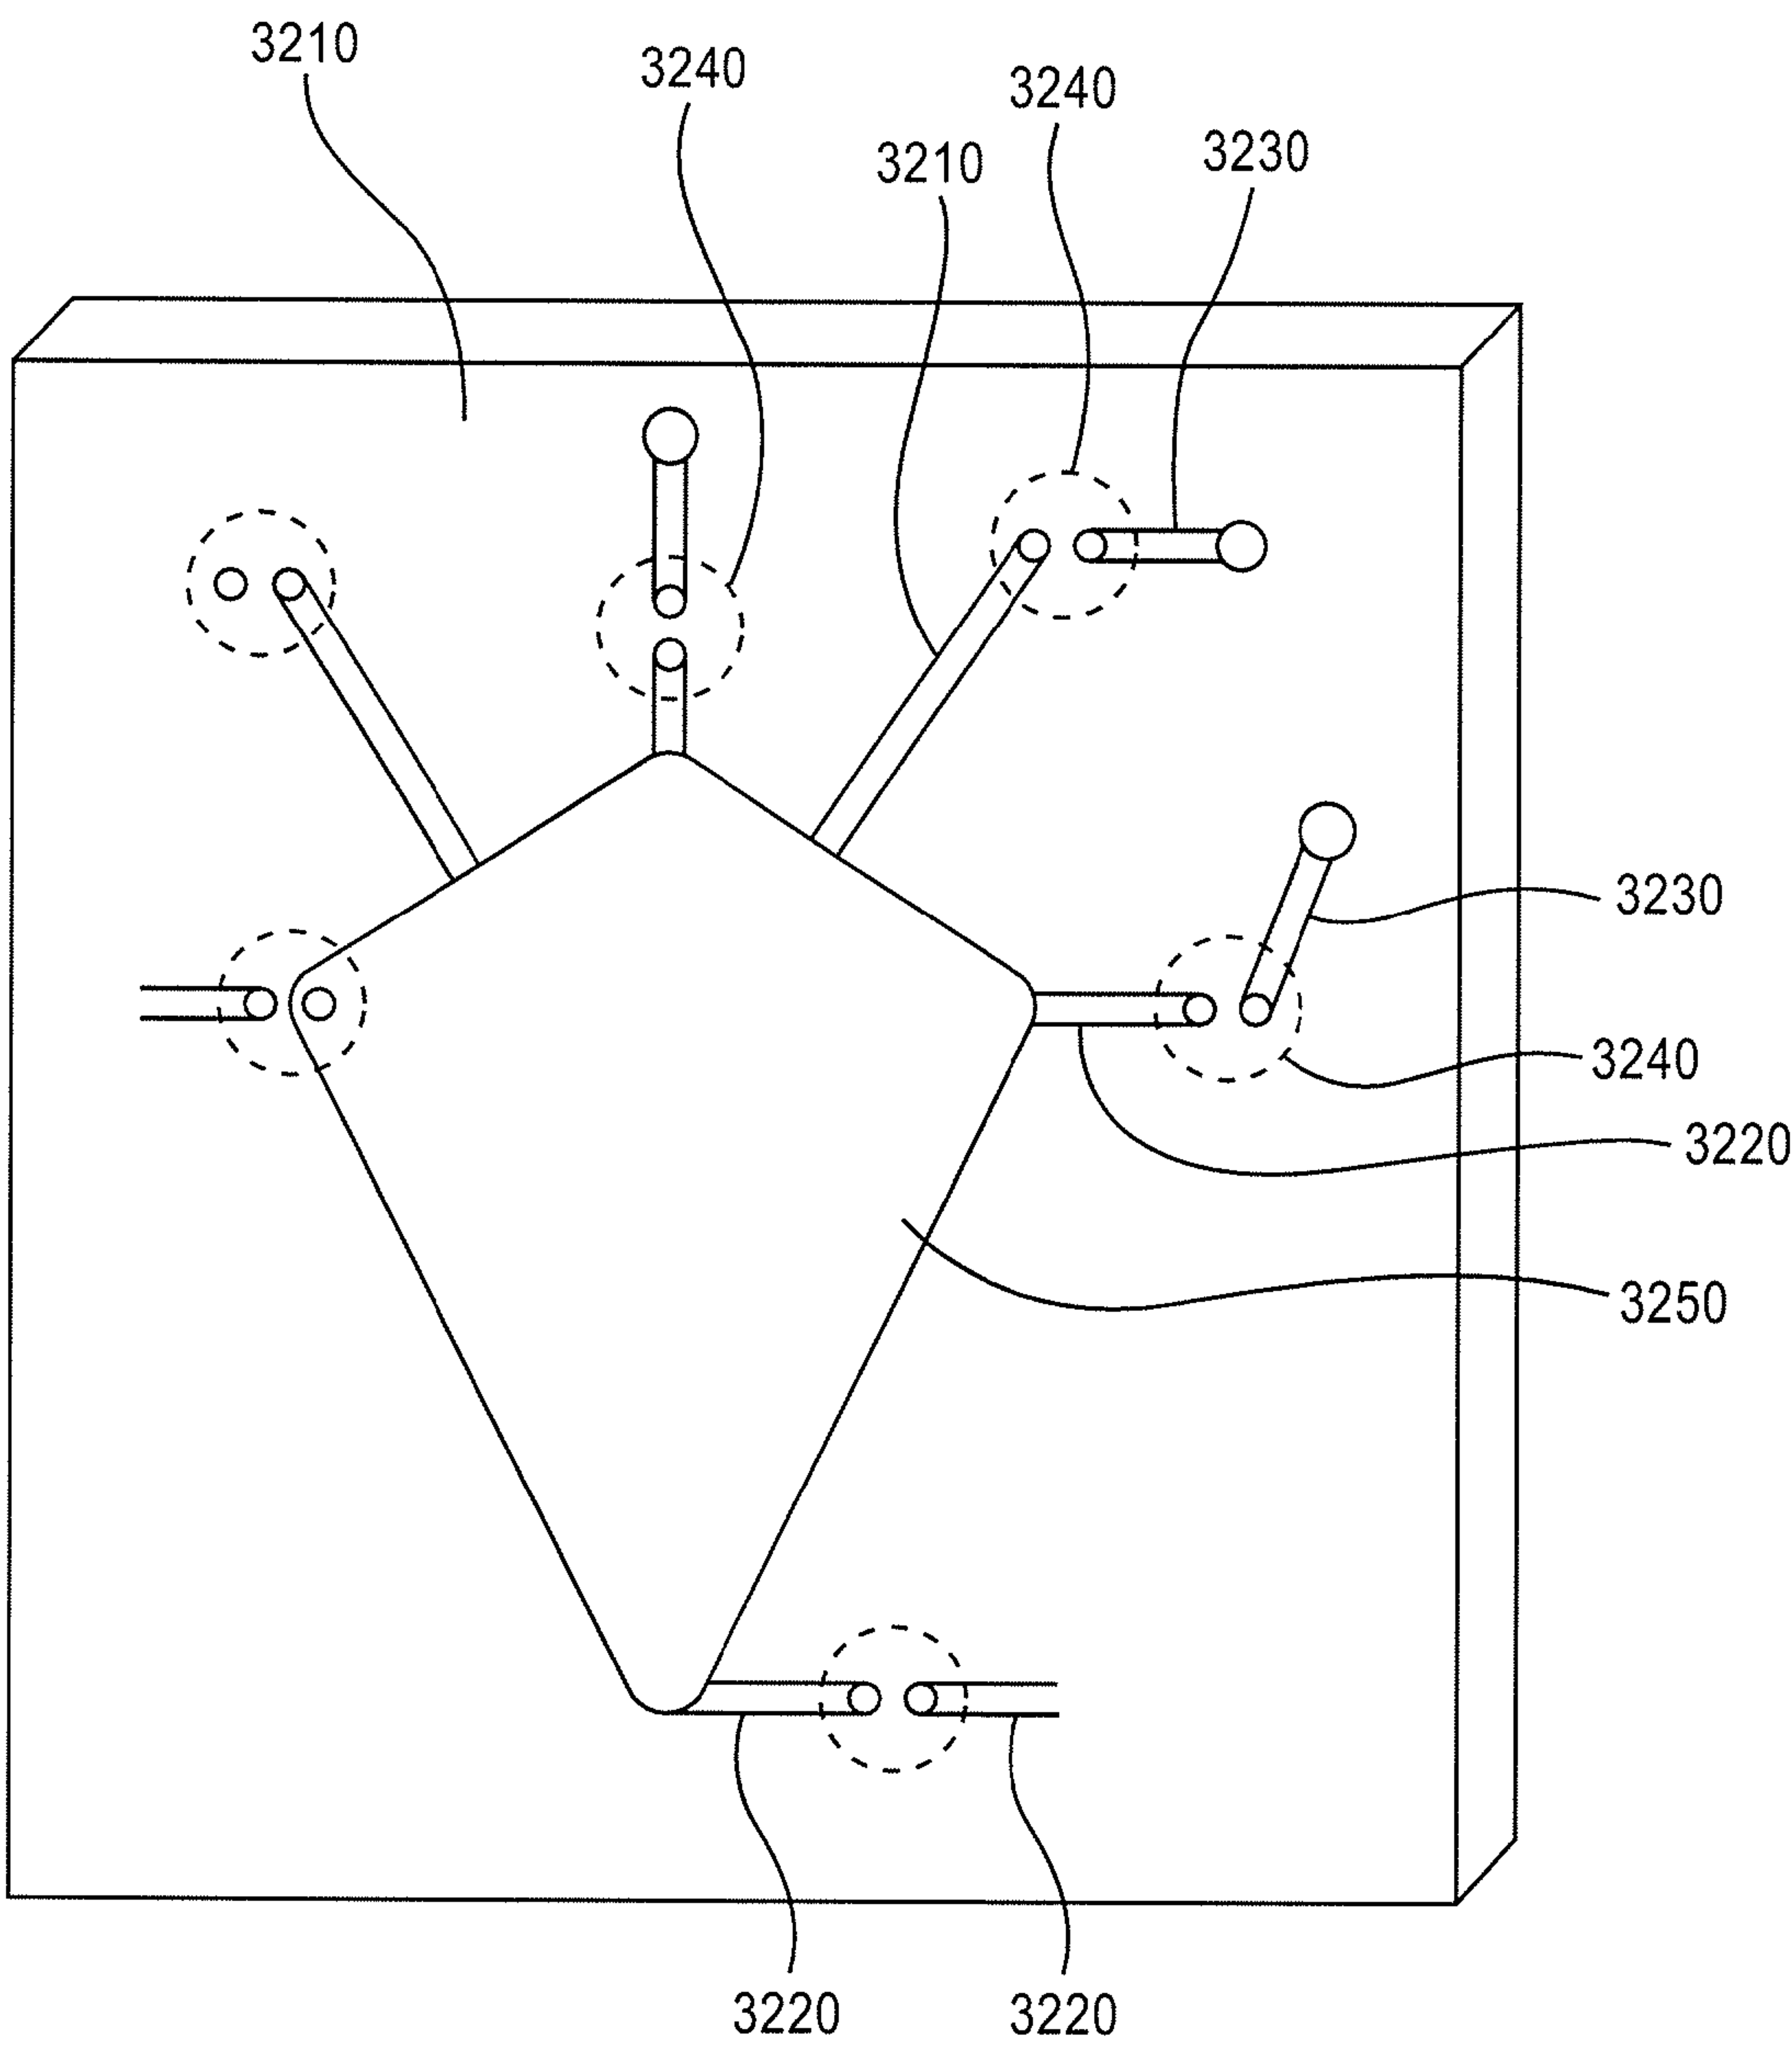


FIG.32

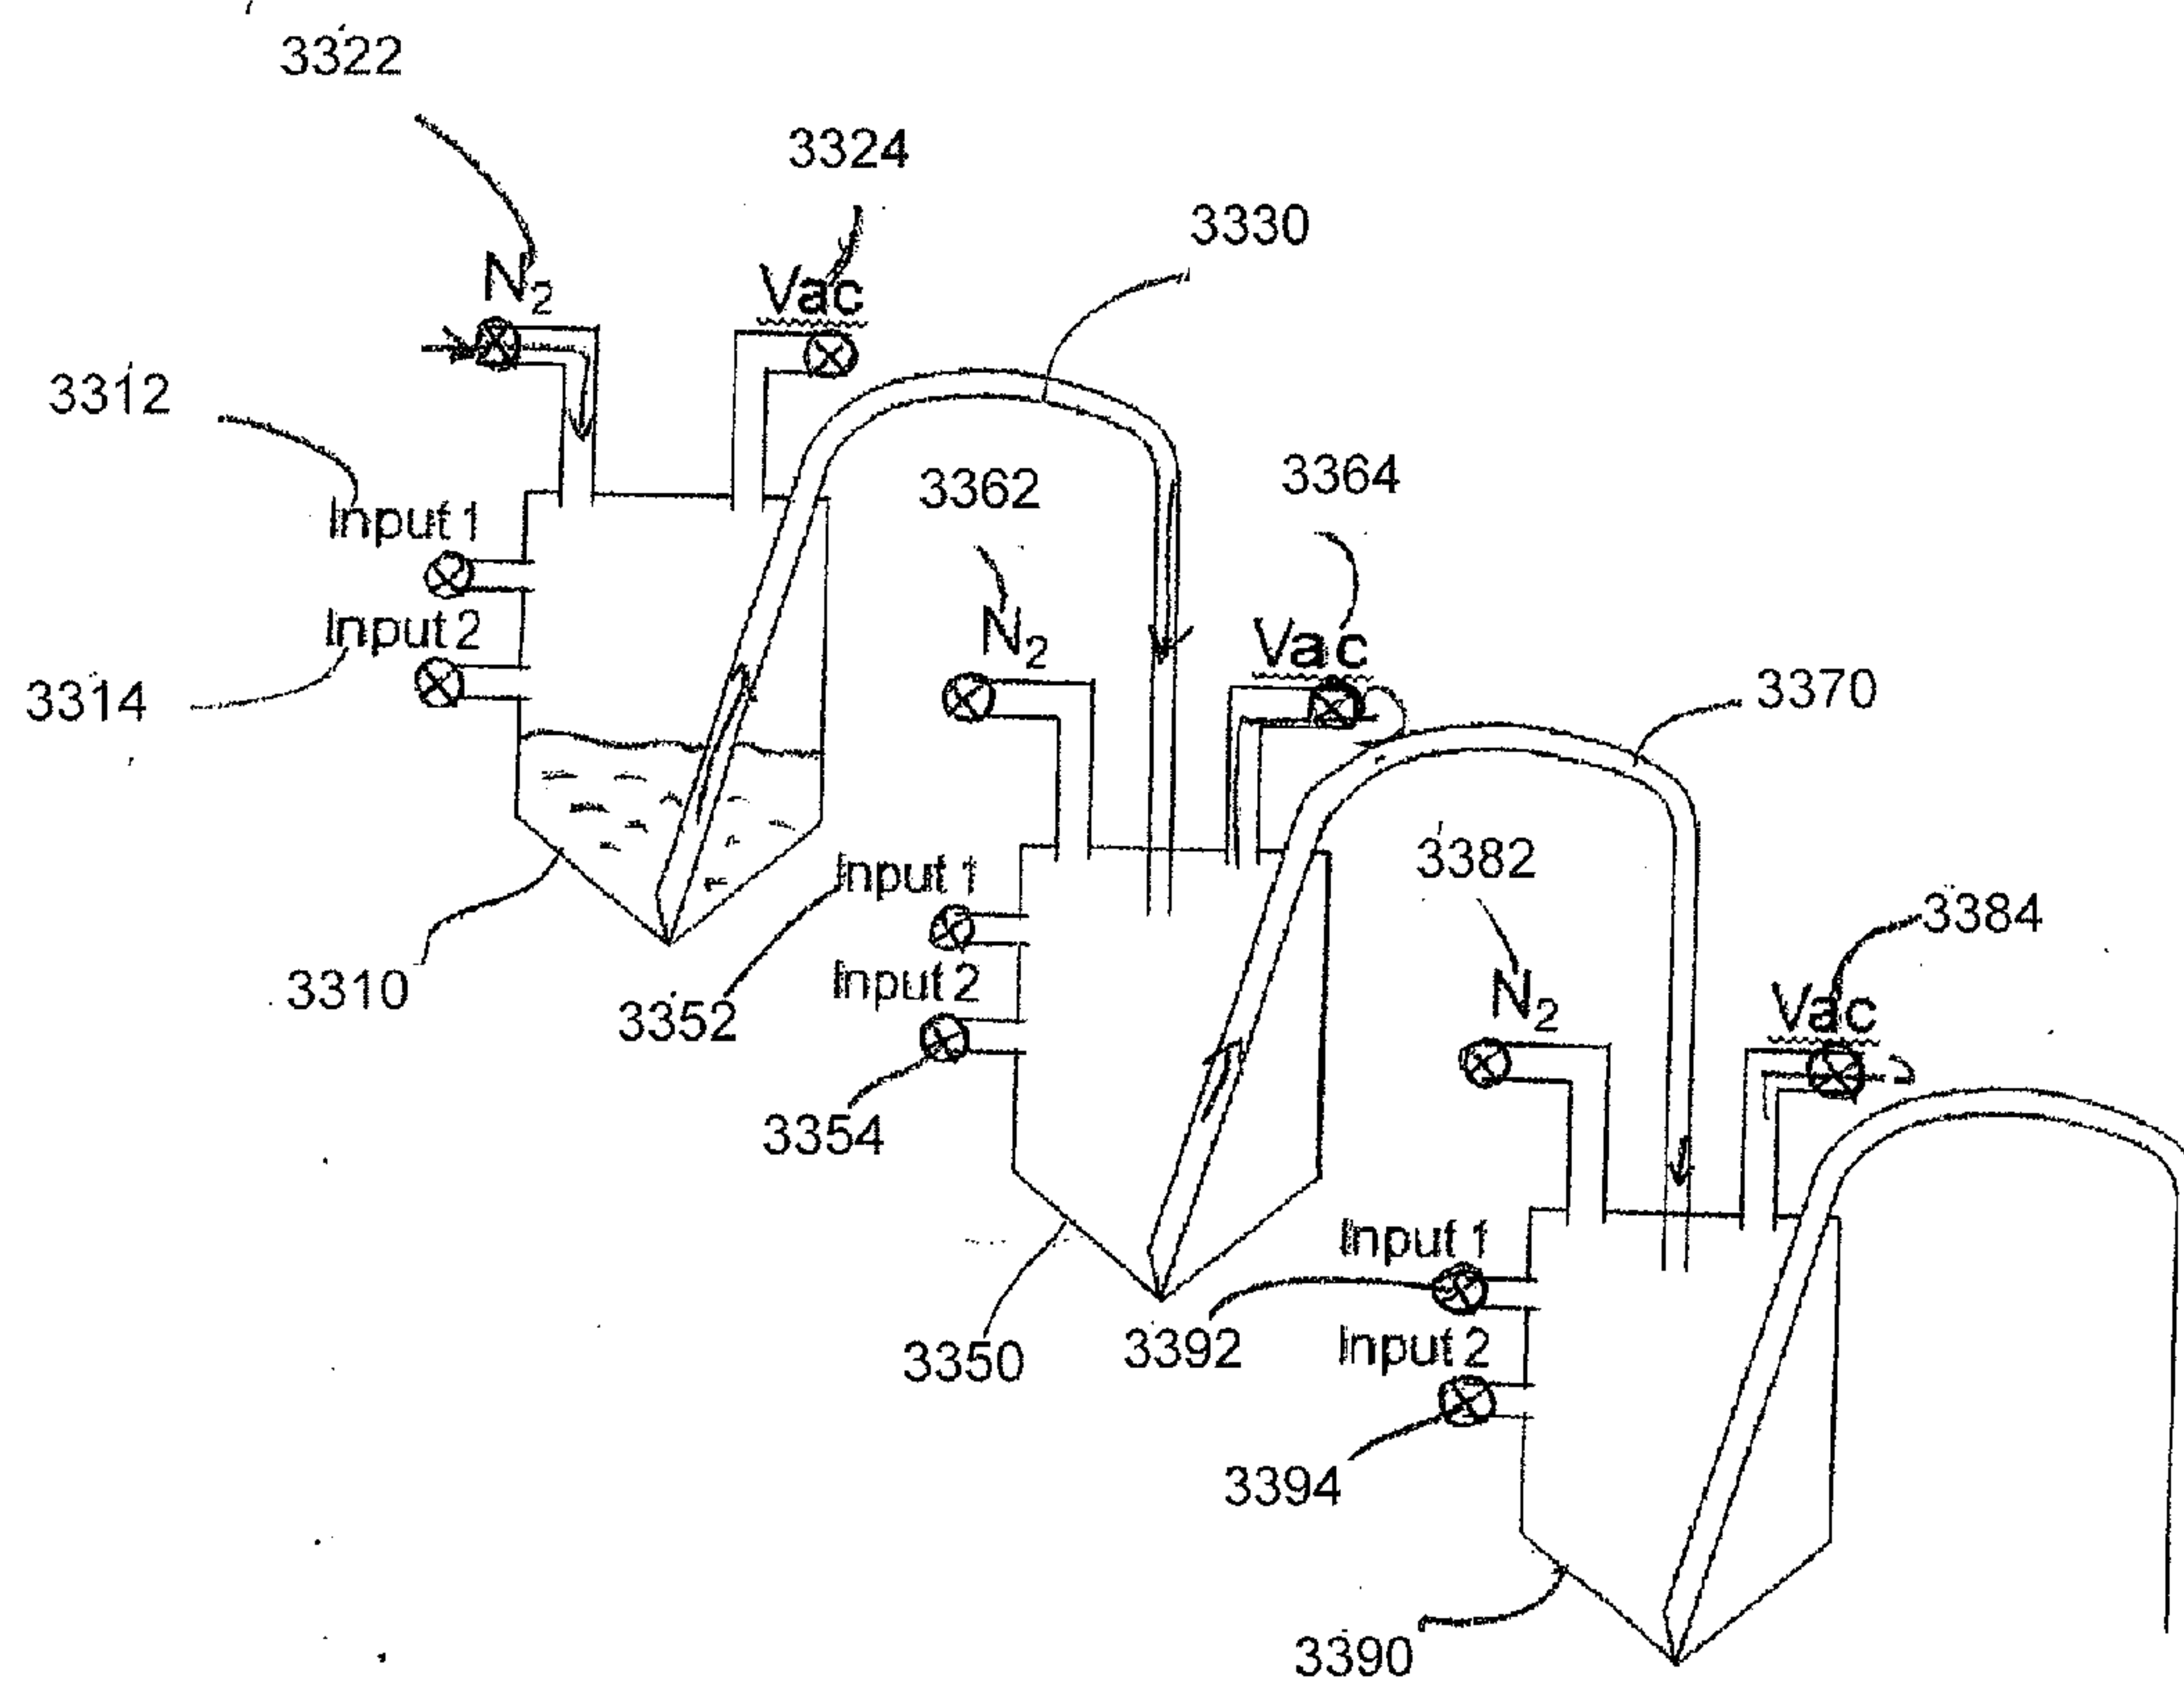


FIG. 33




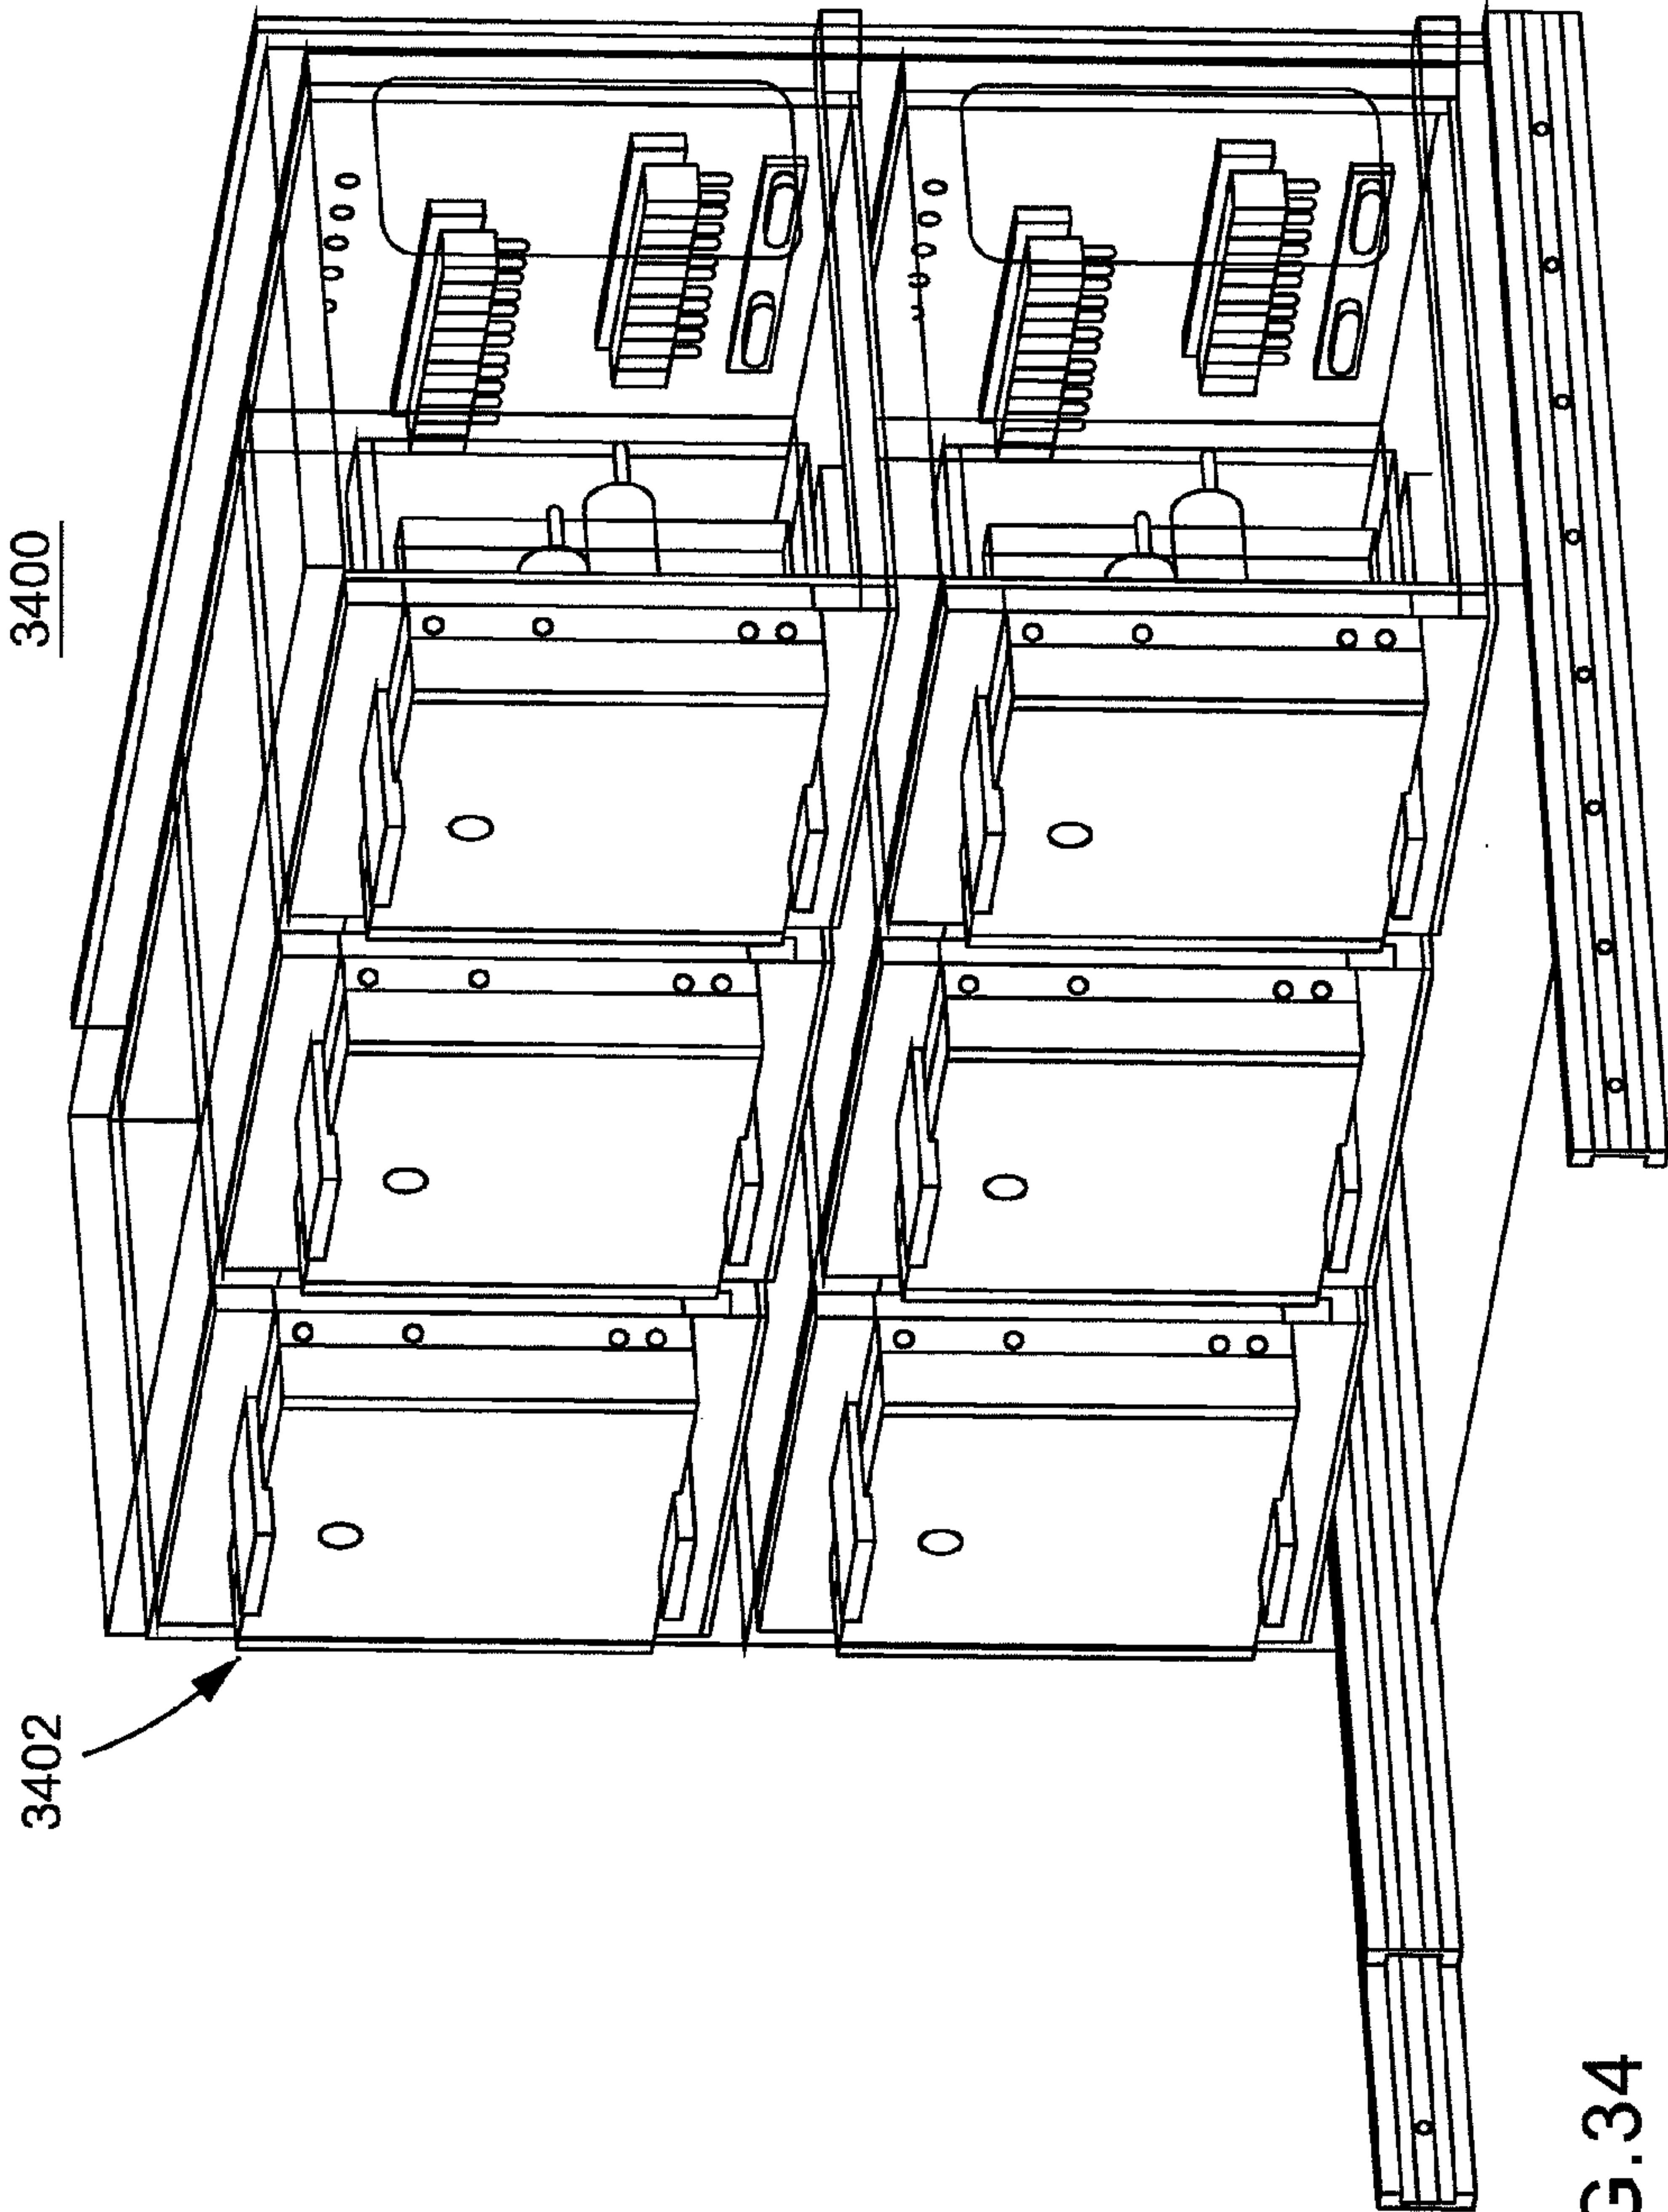


FIG. 34

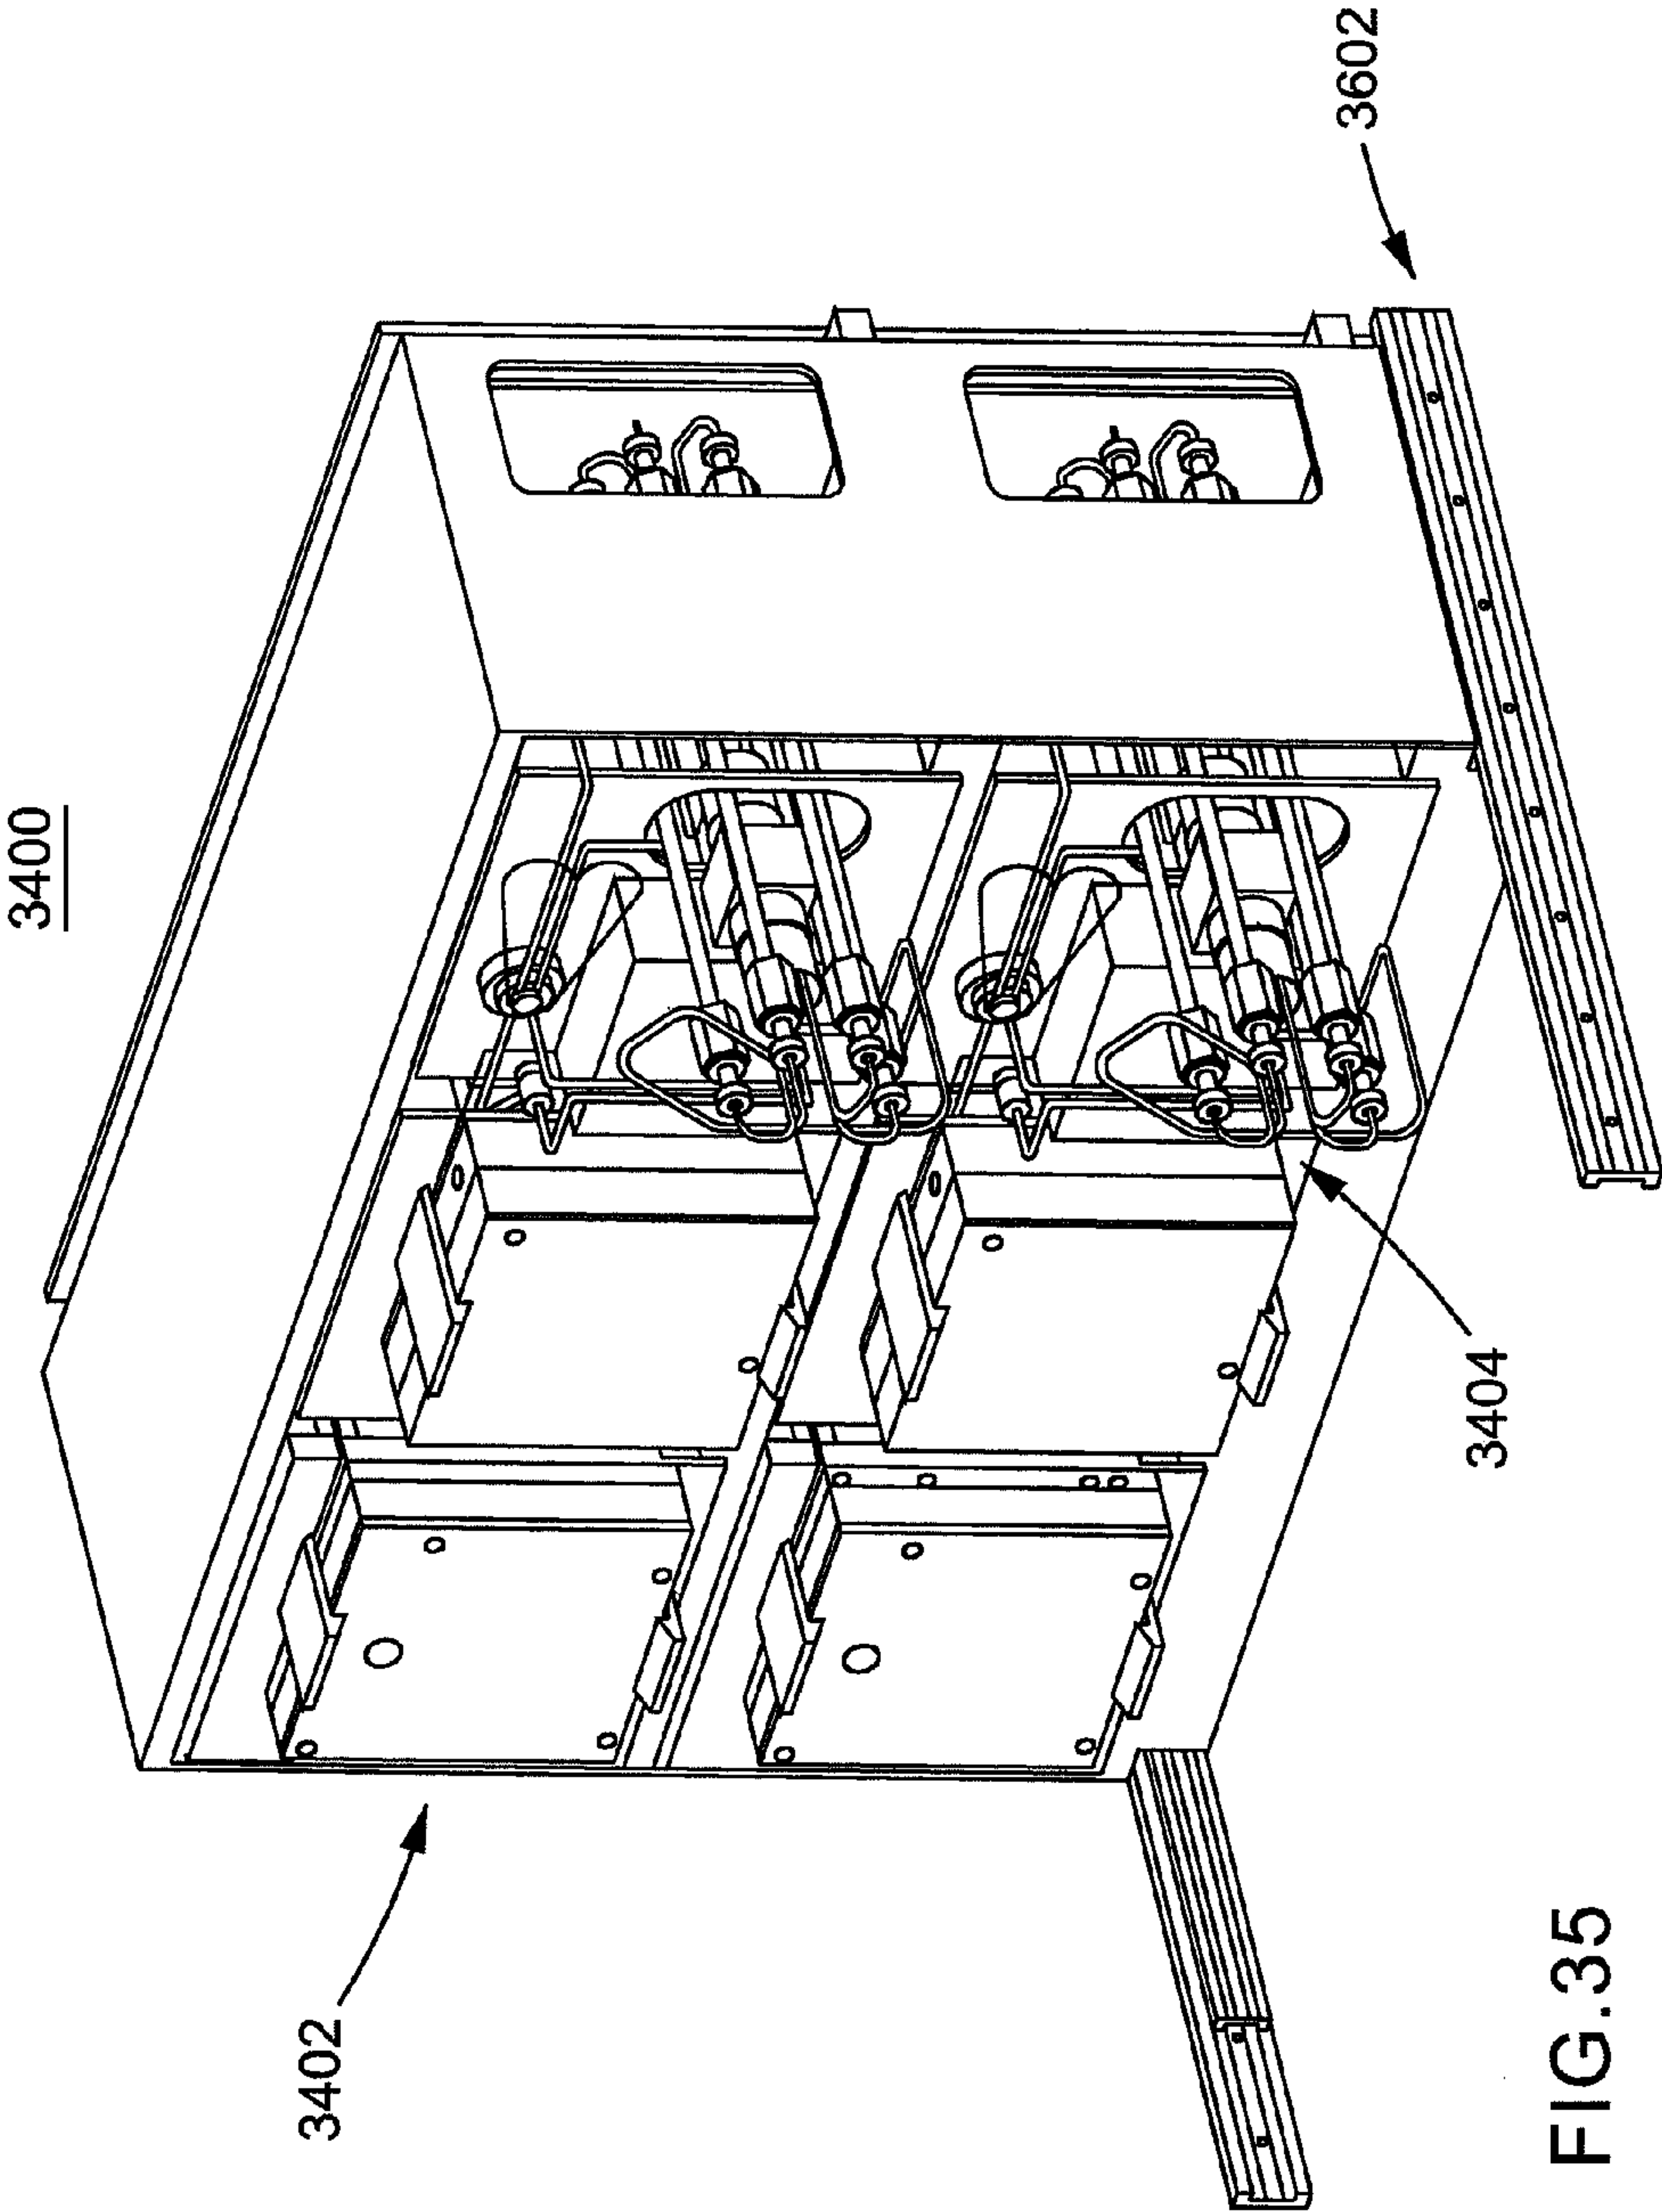



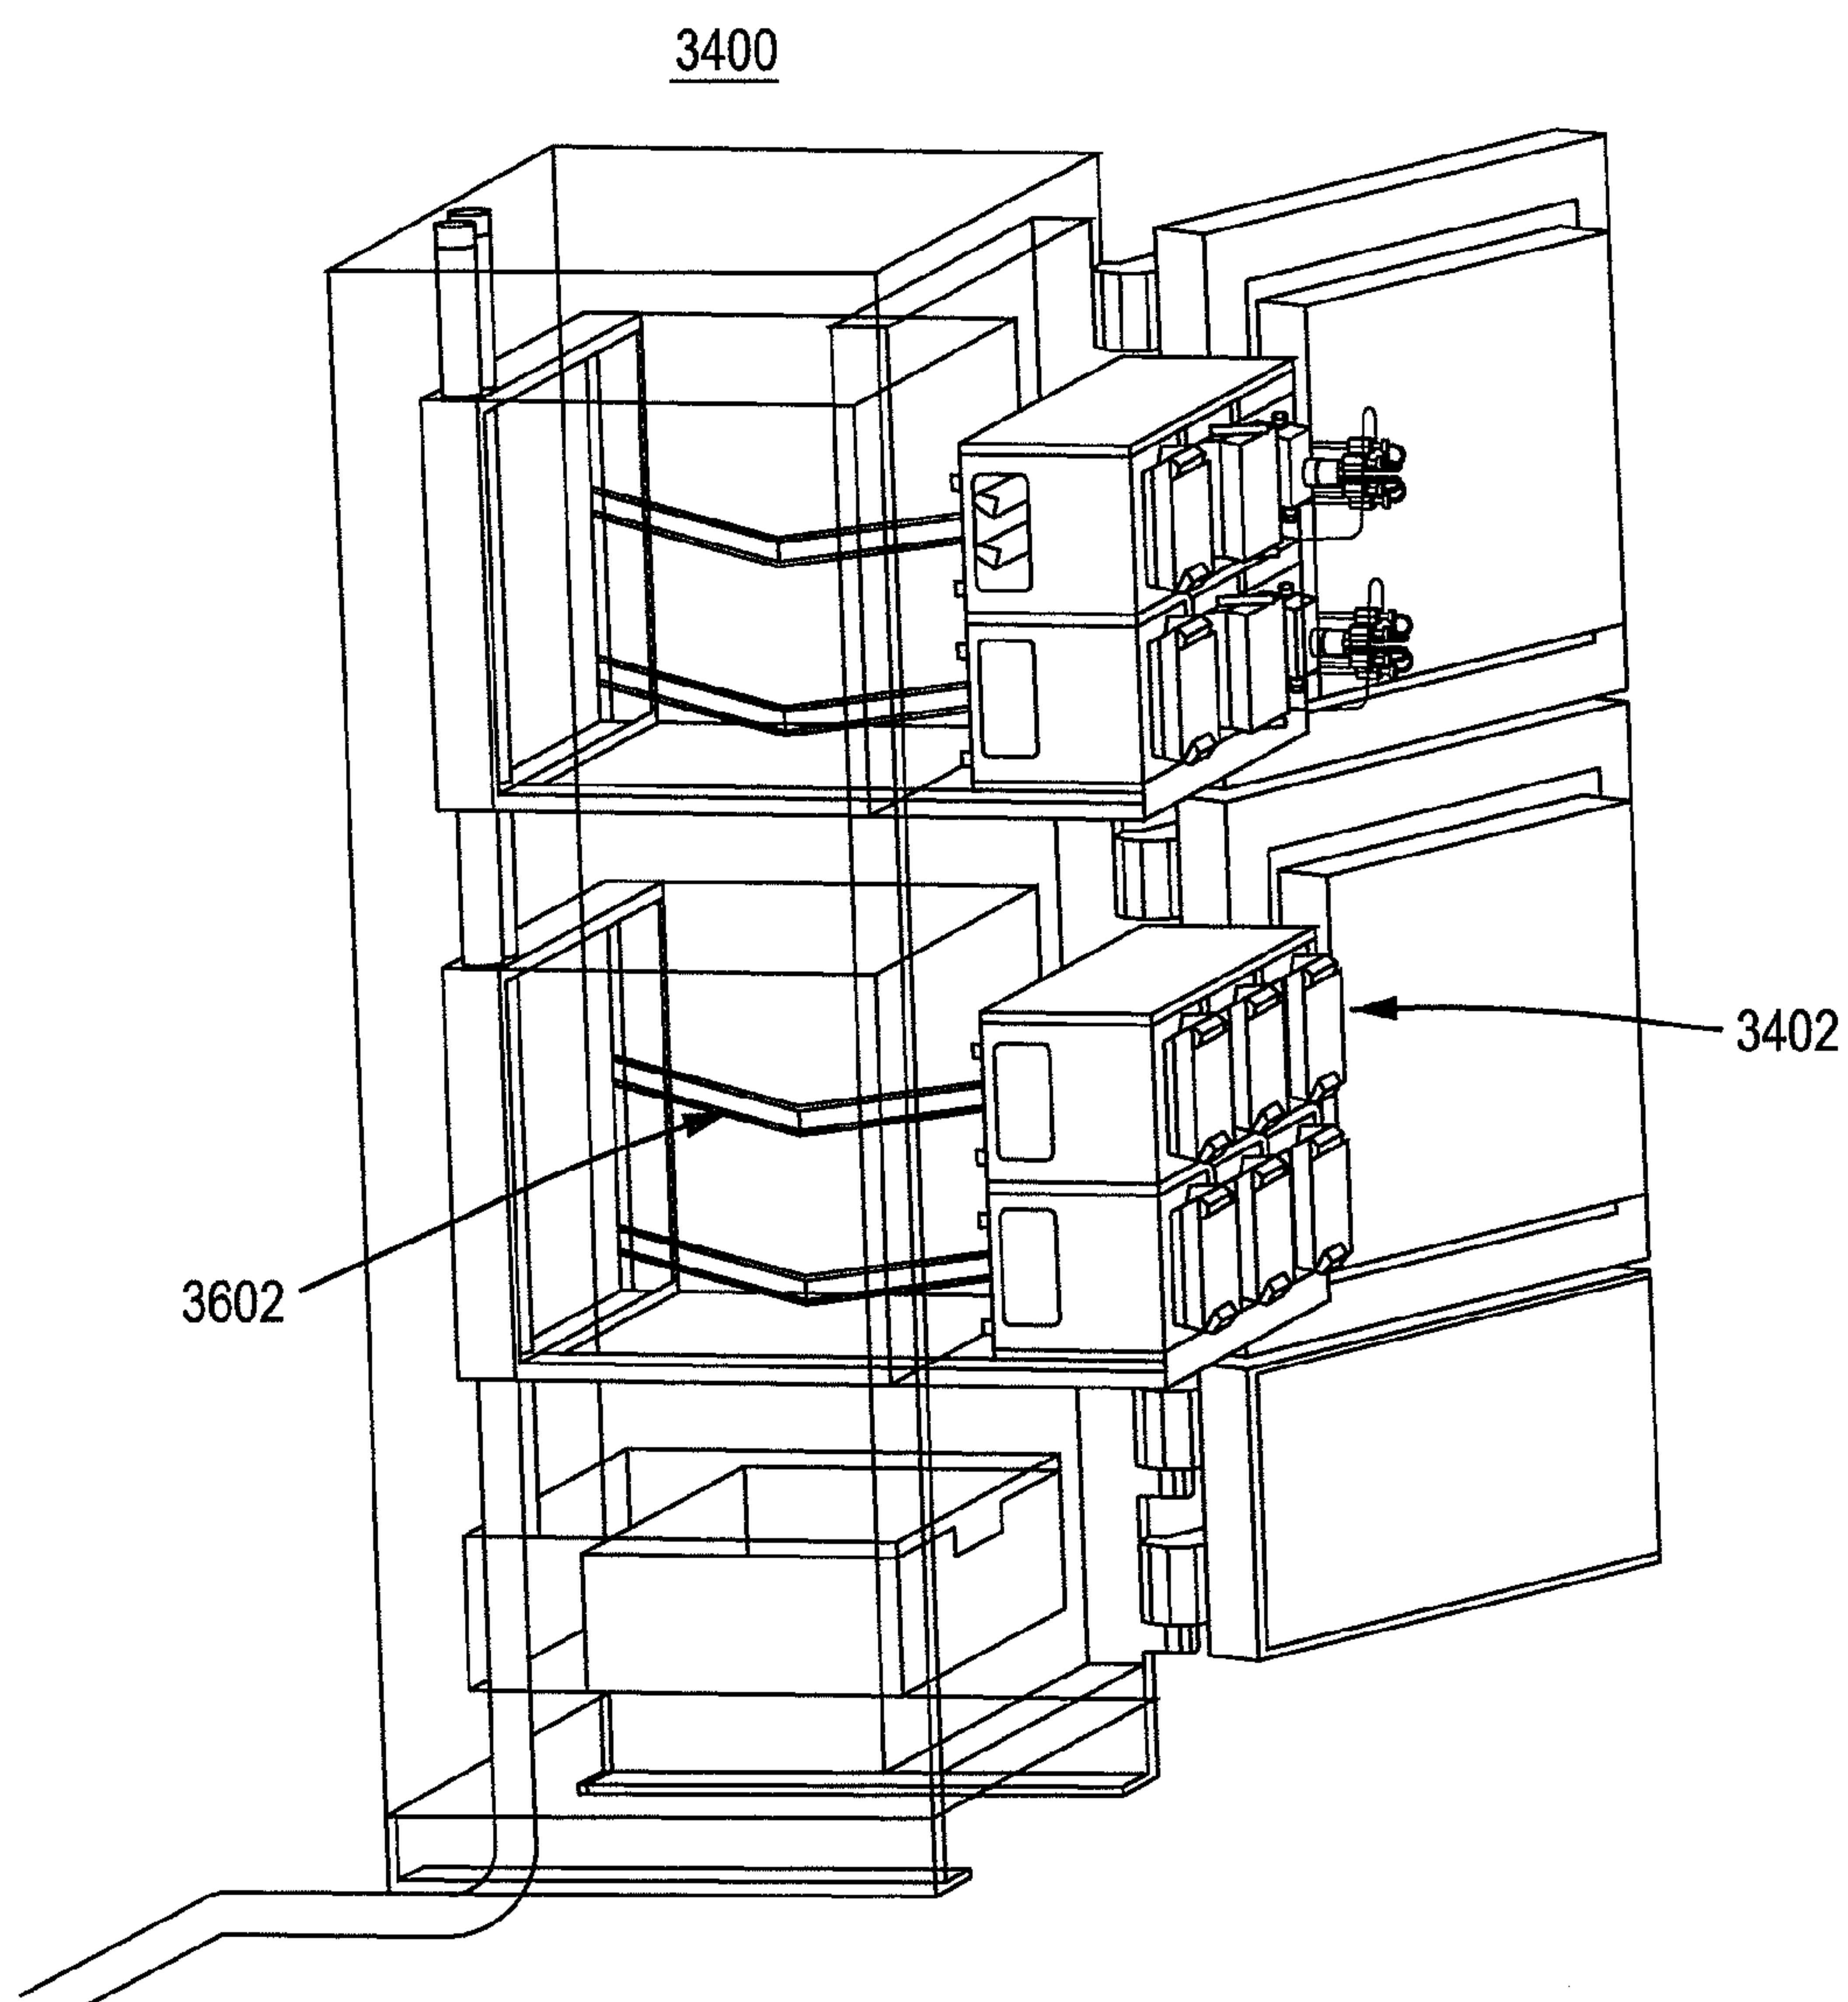


Fig.36

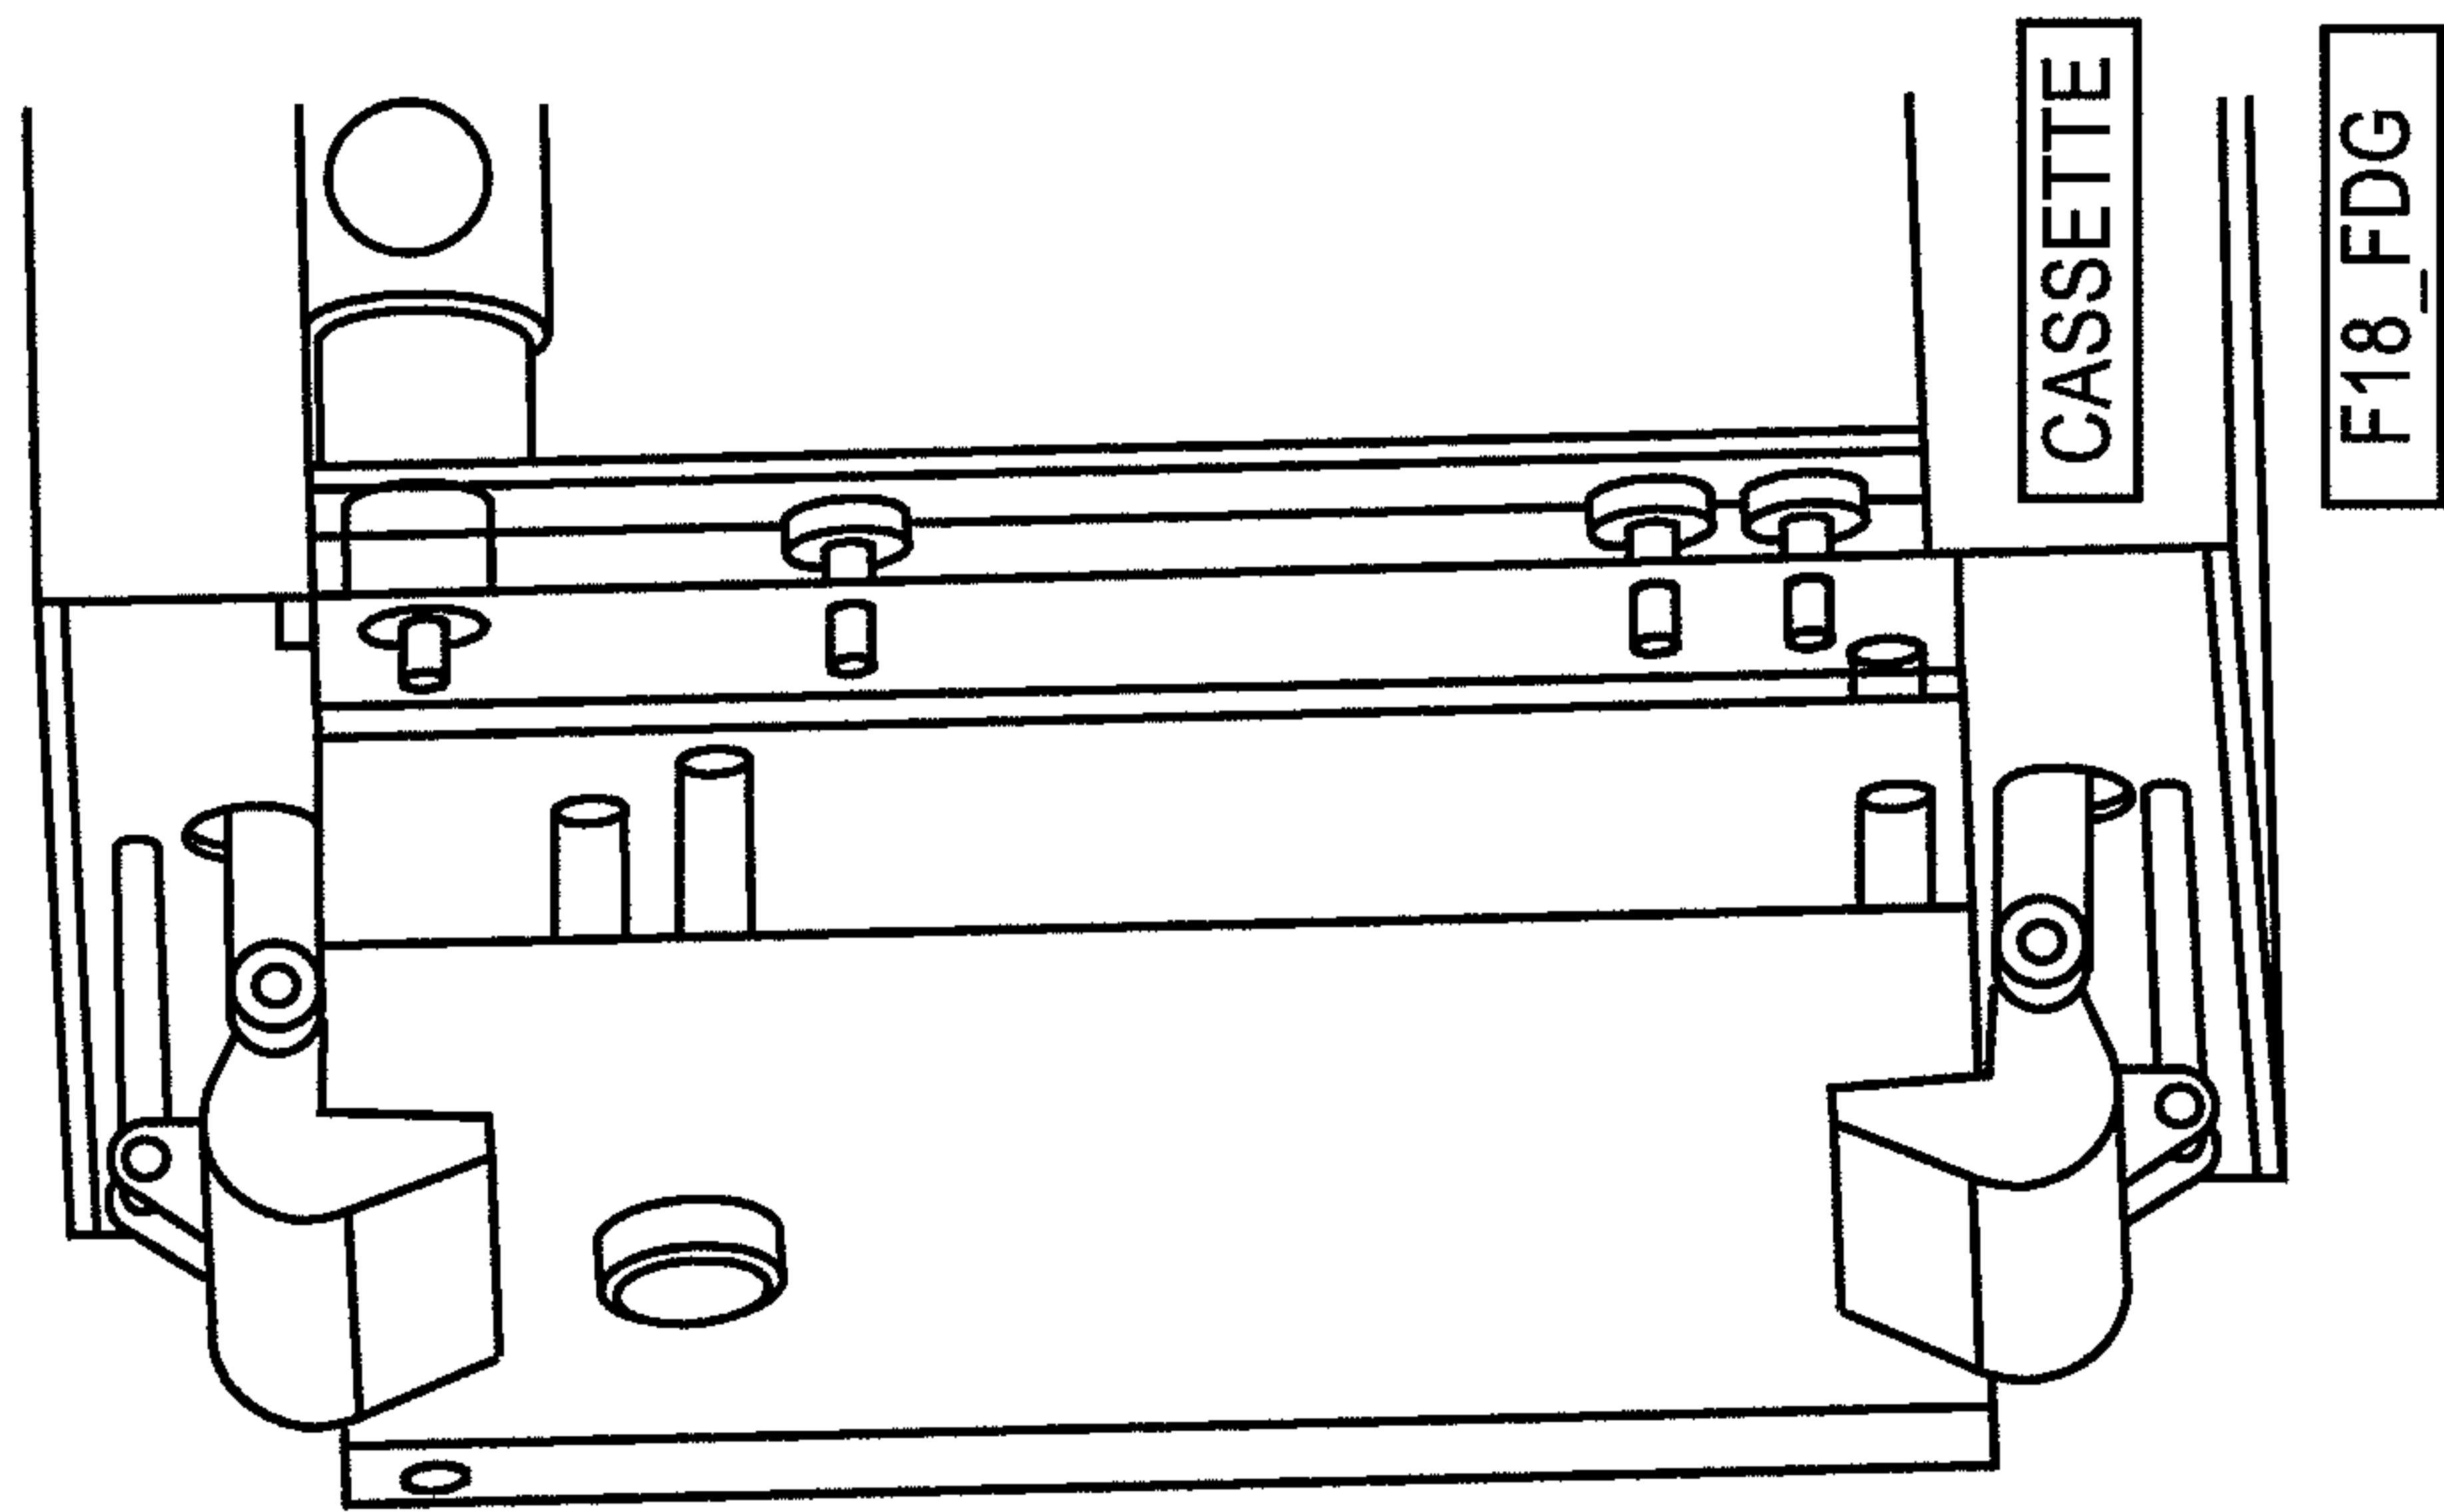


FIG.37



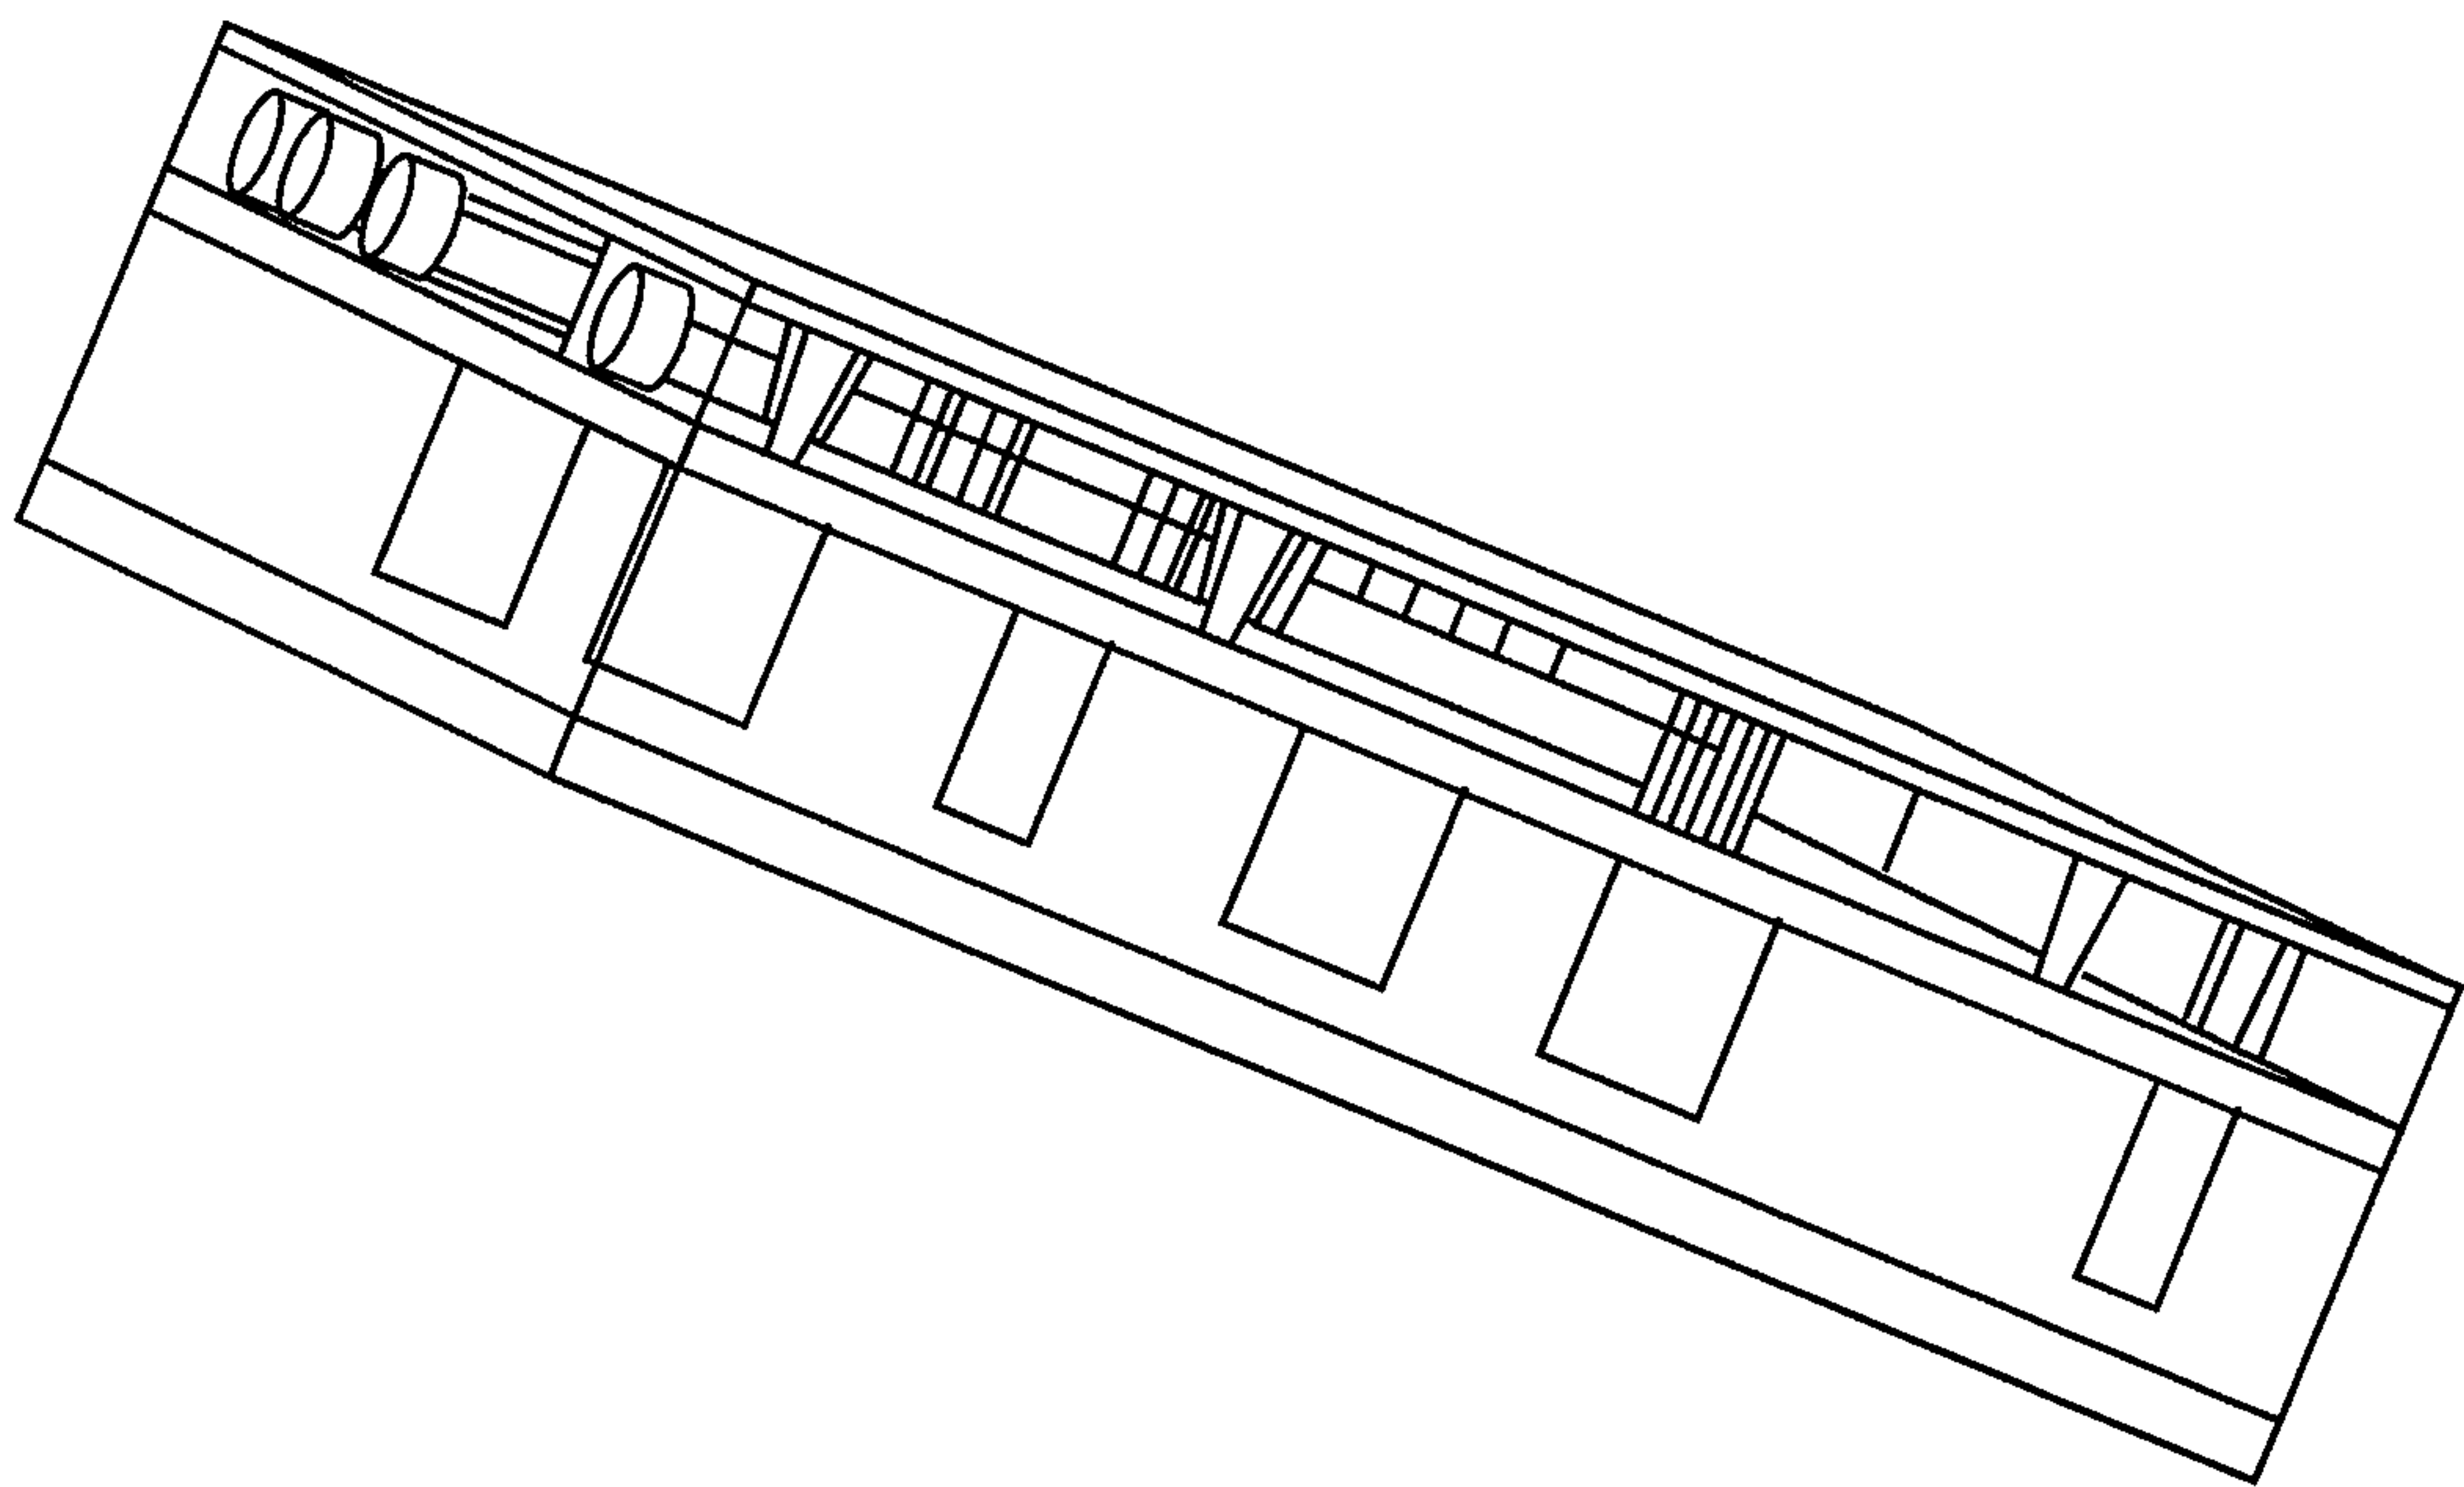


FIG. 38

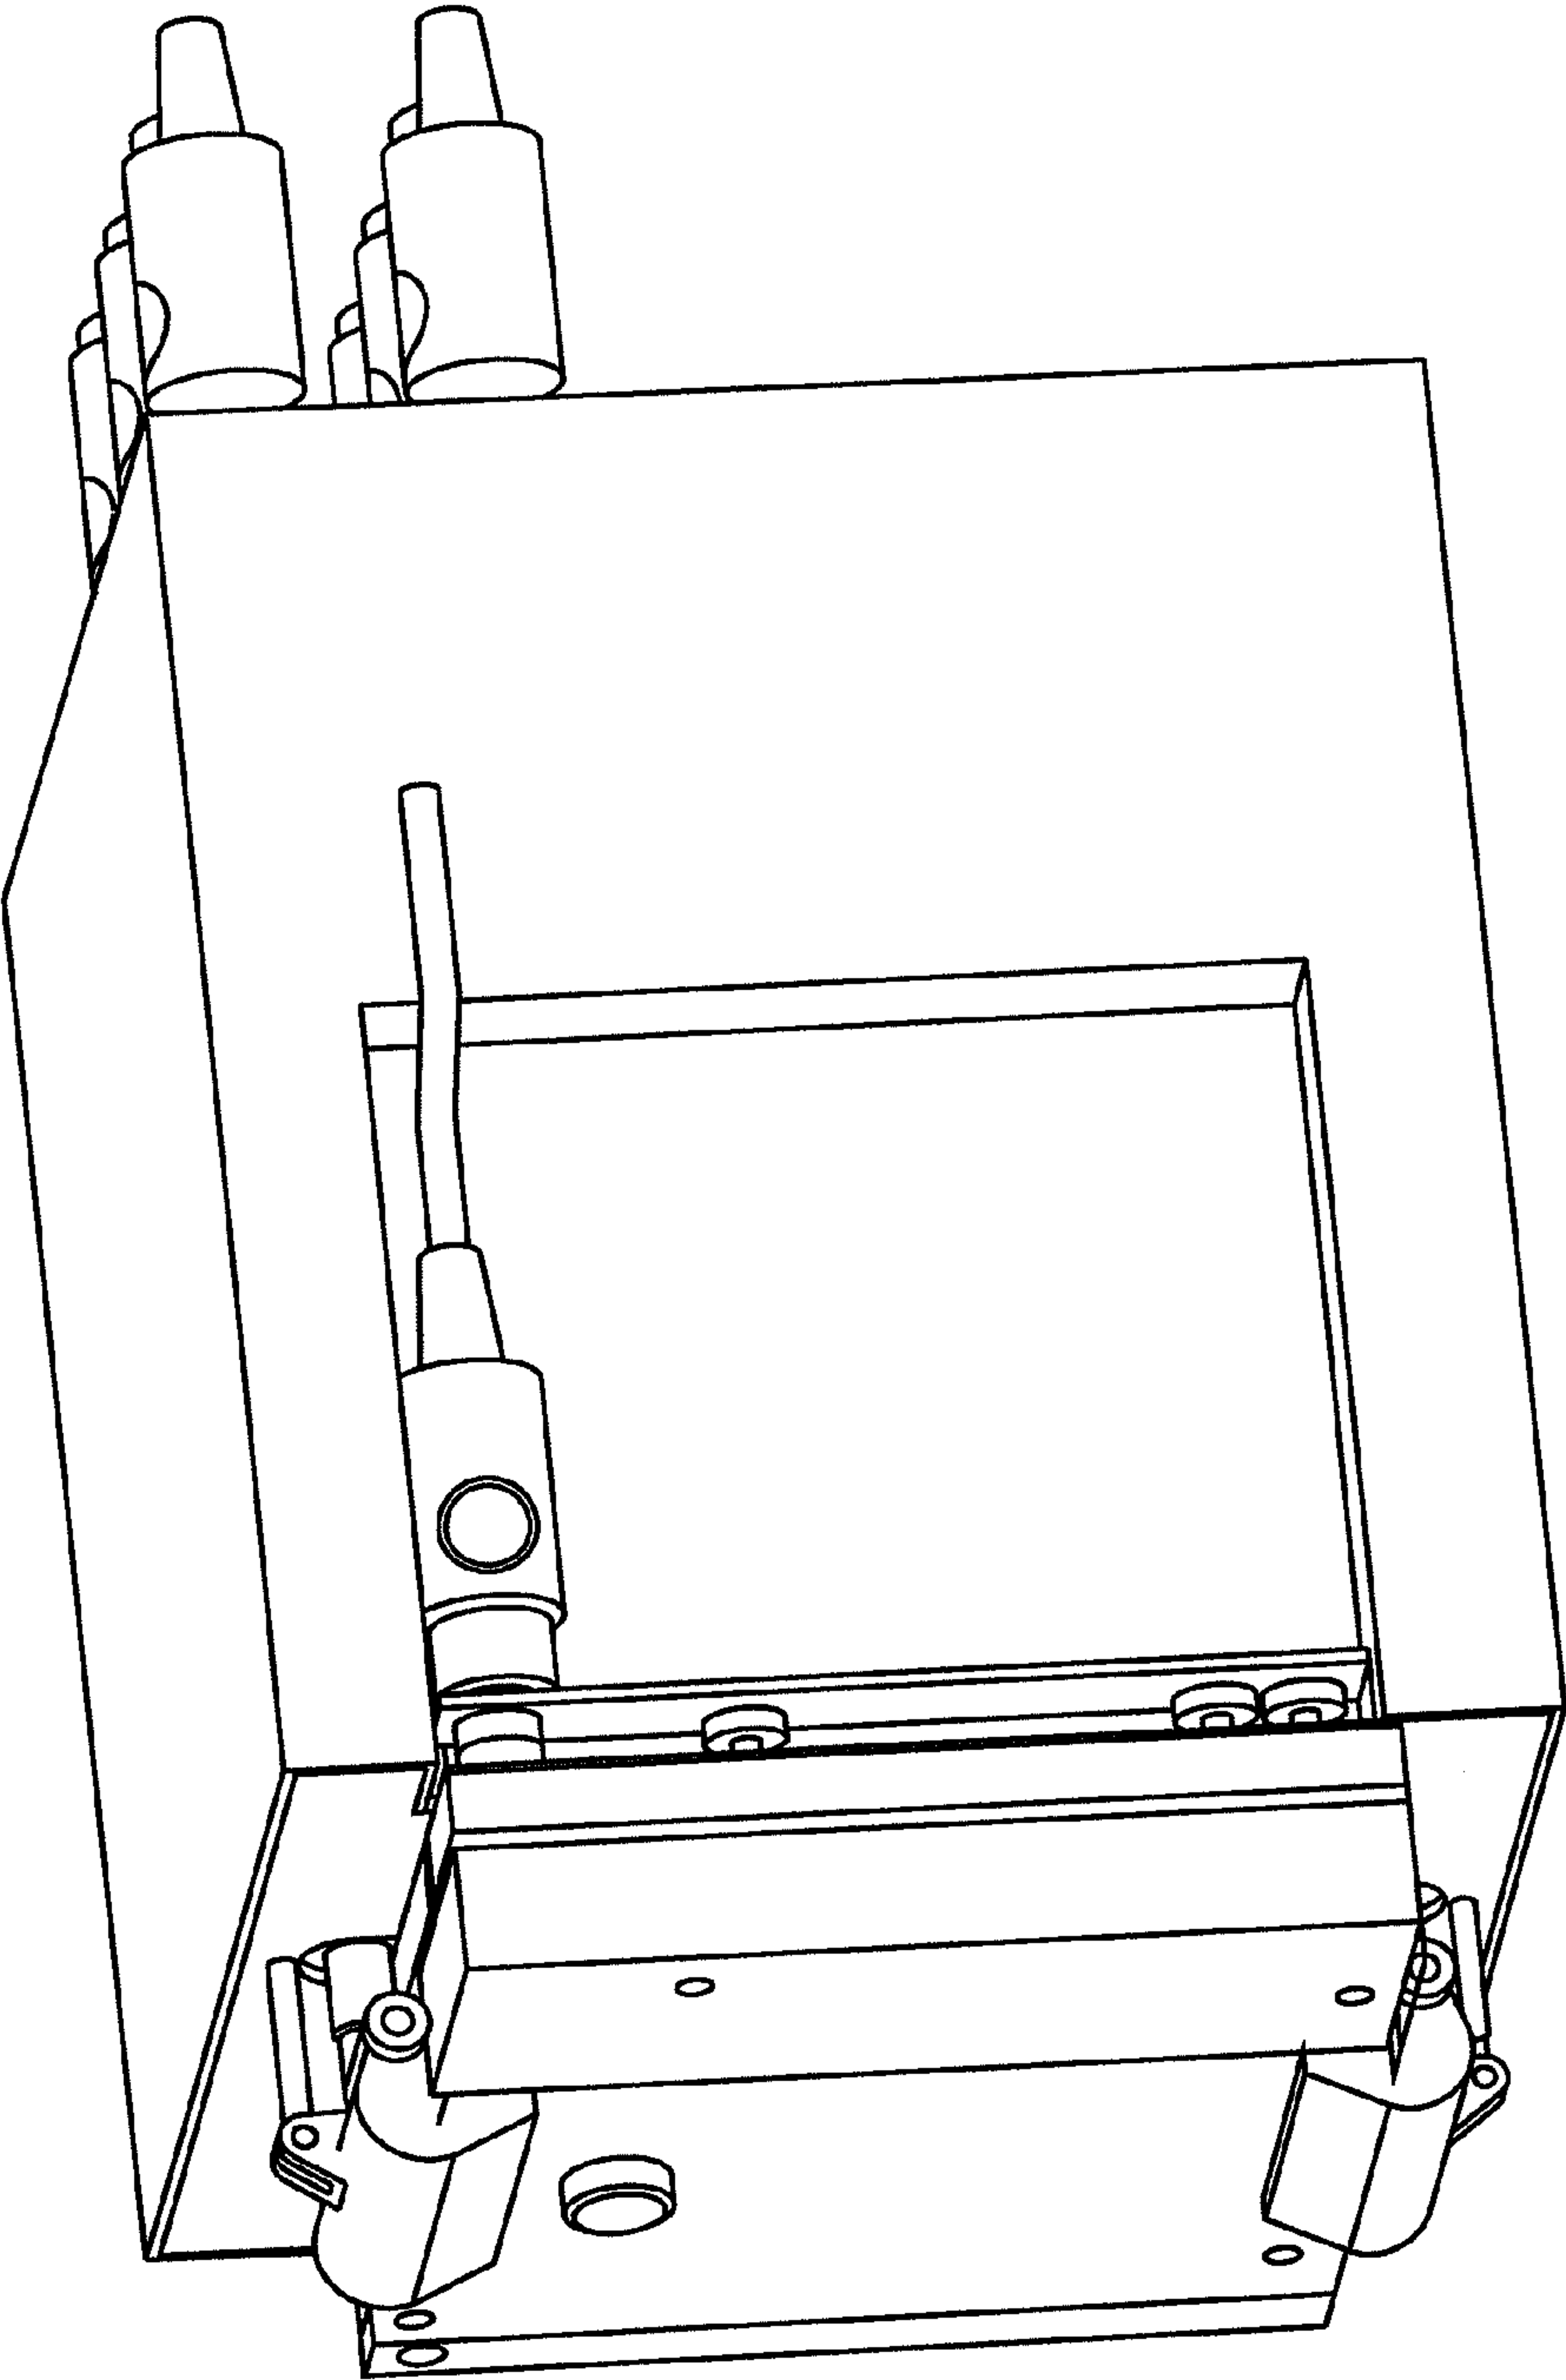


FIG.39



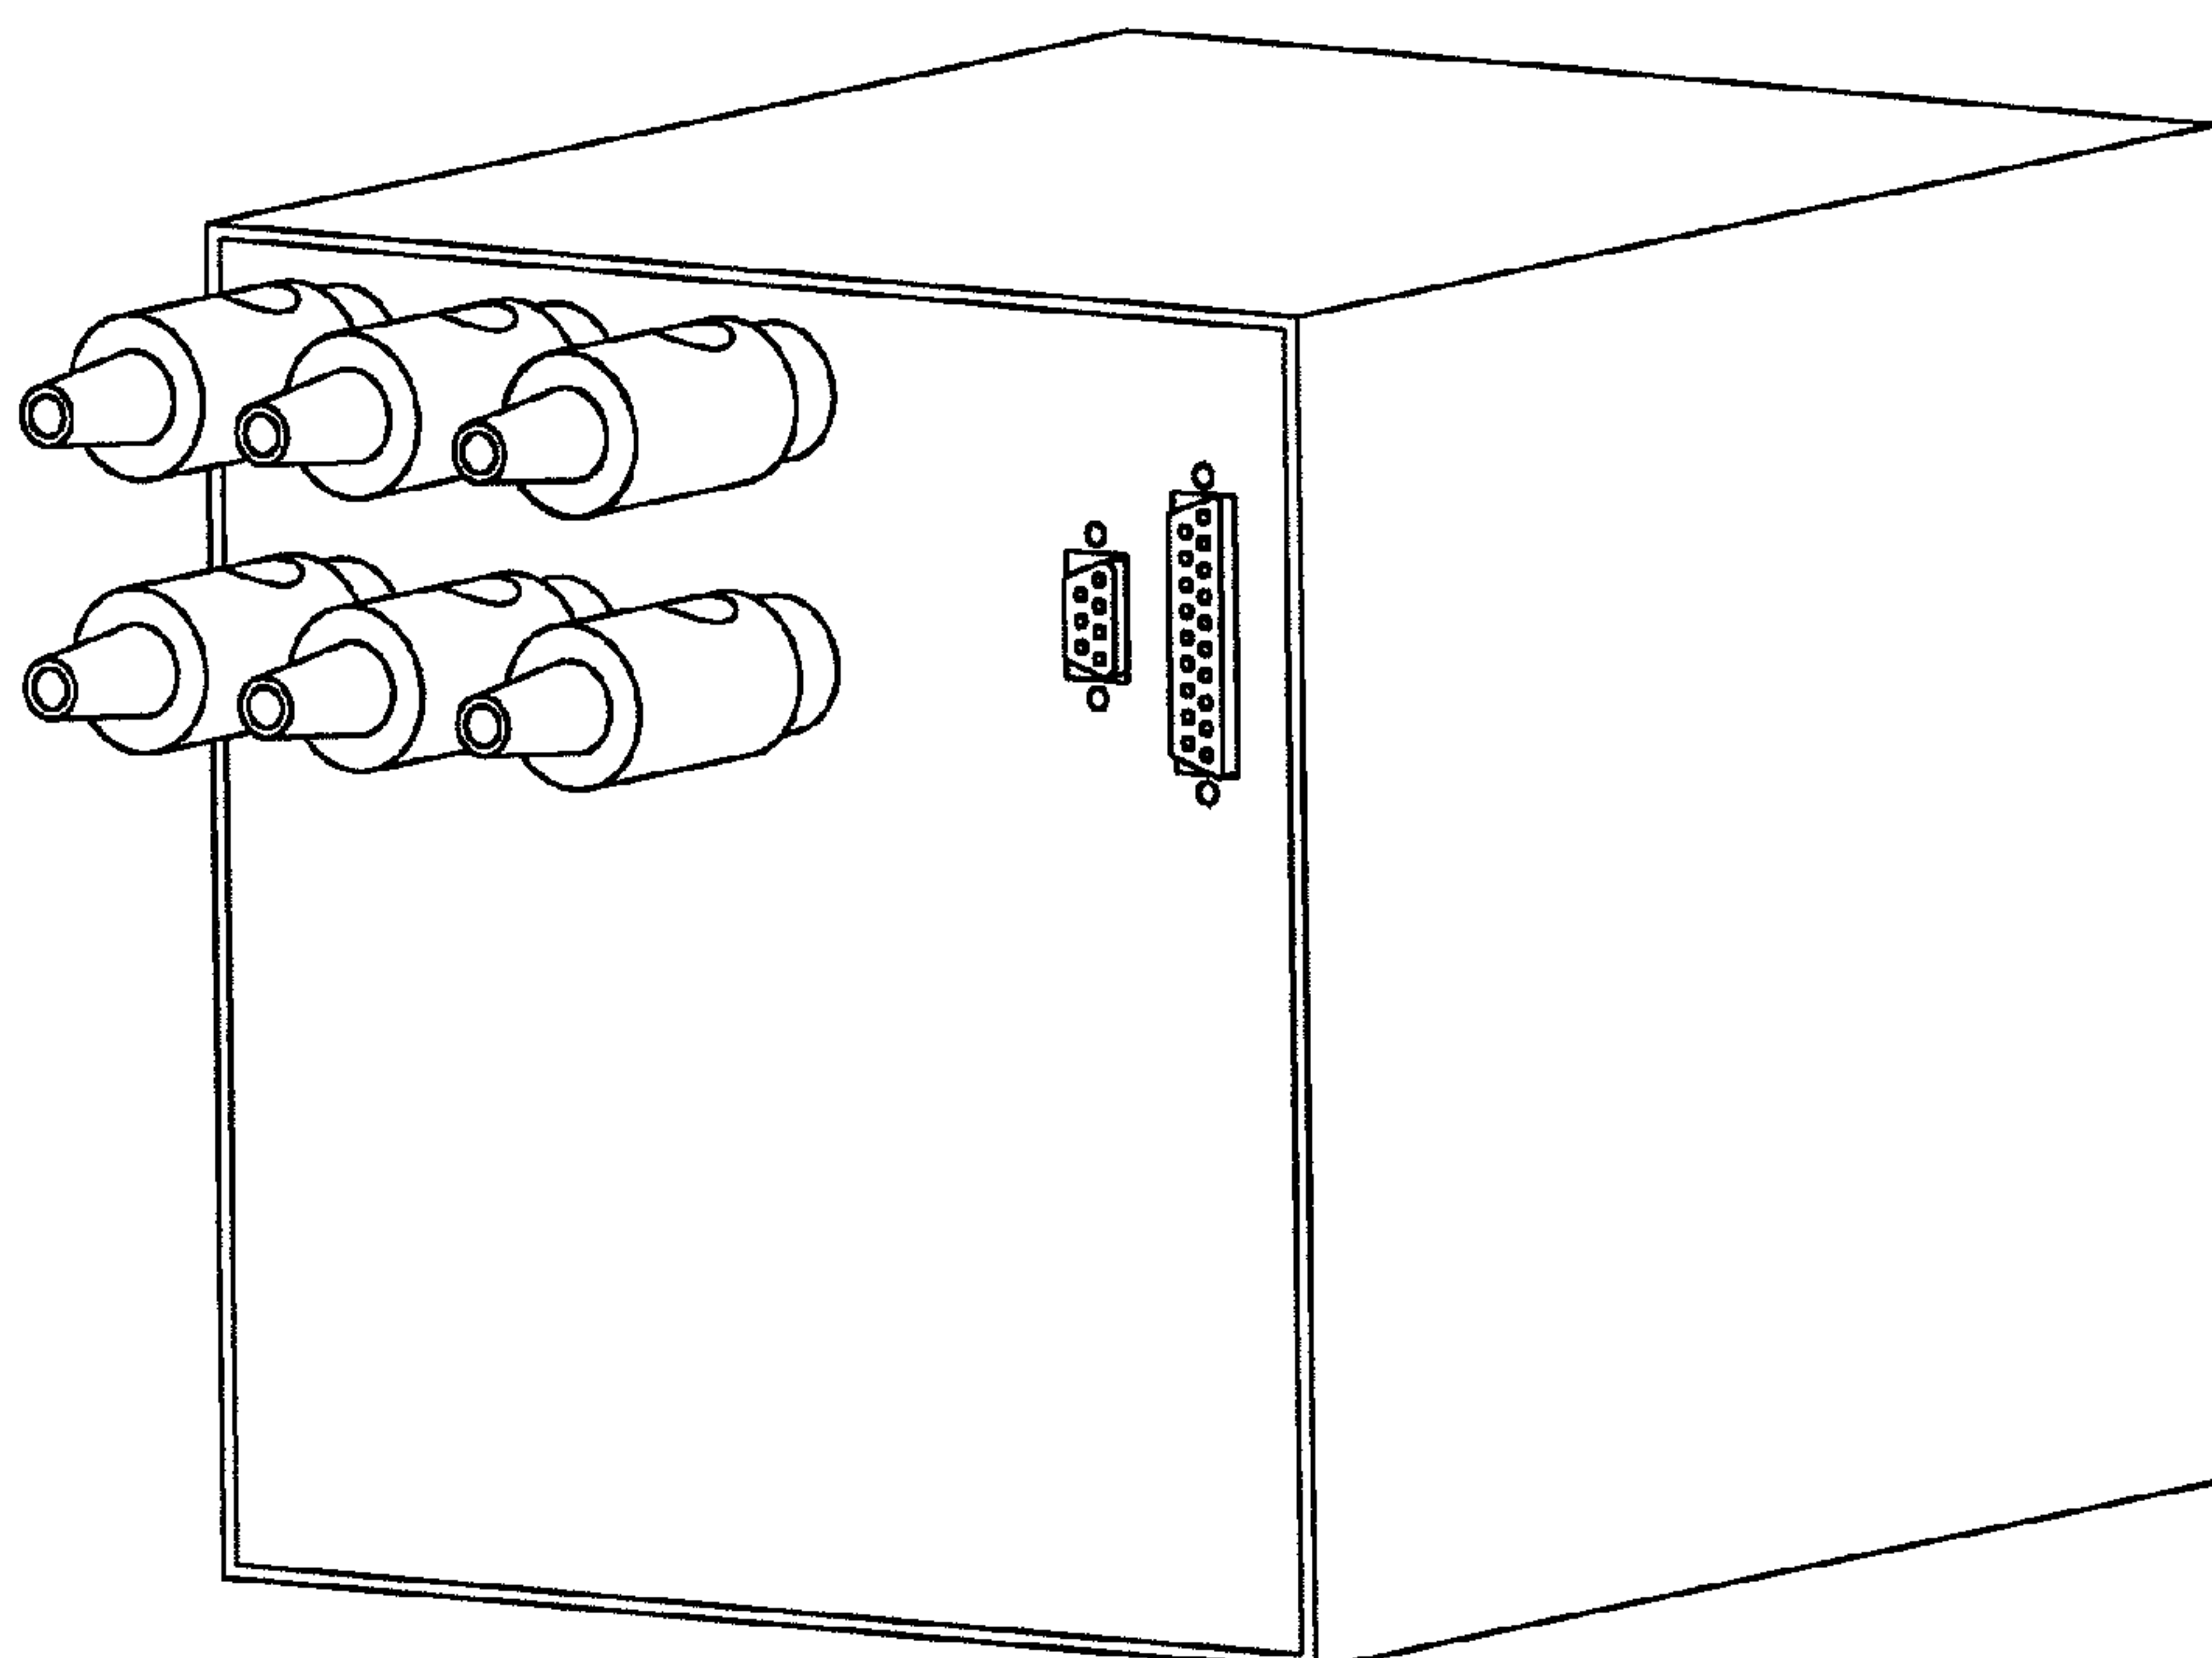


FIG.40a

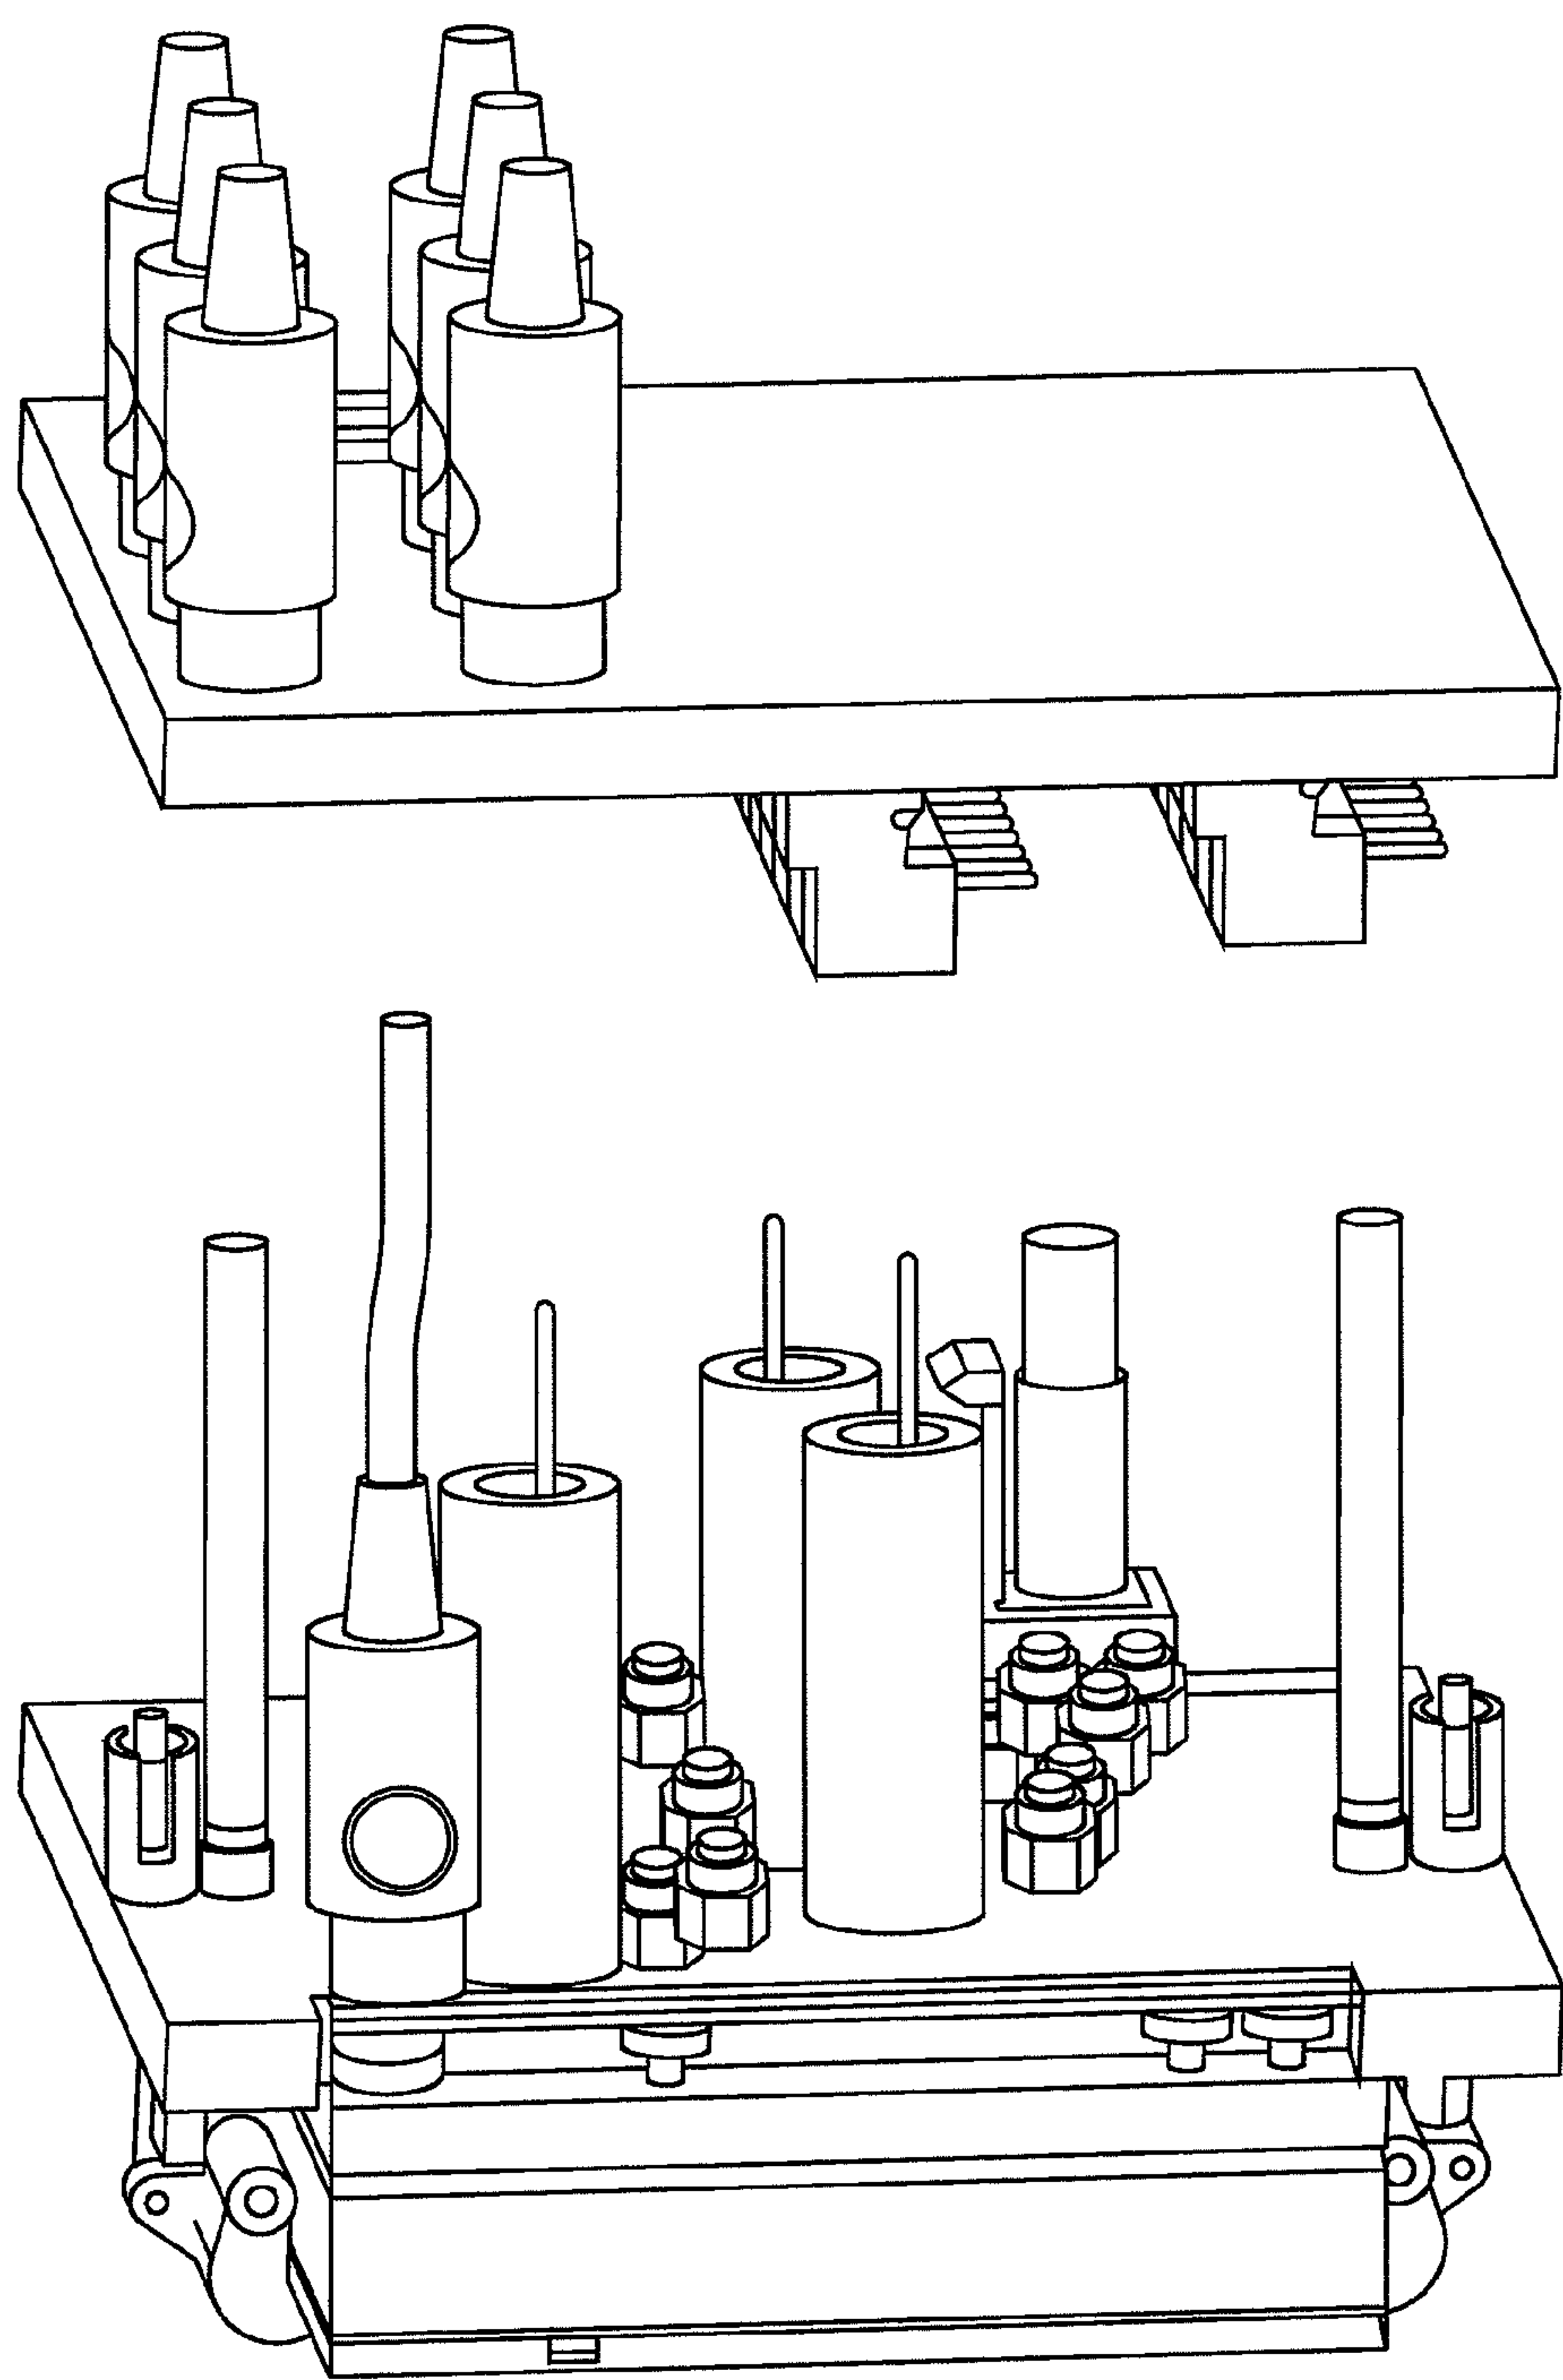


FIG. 40b



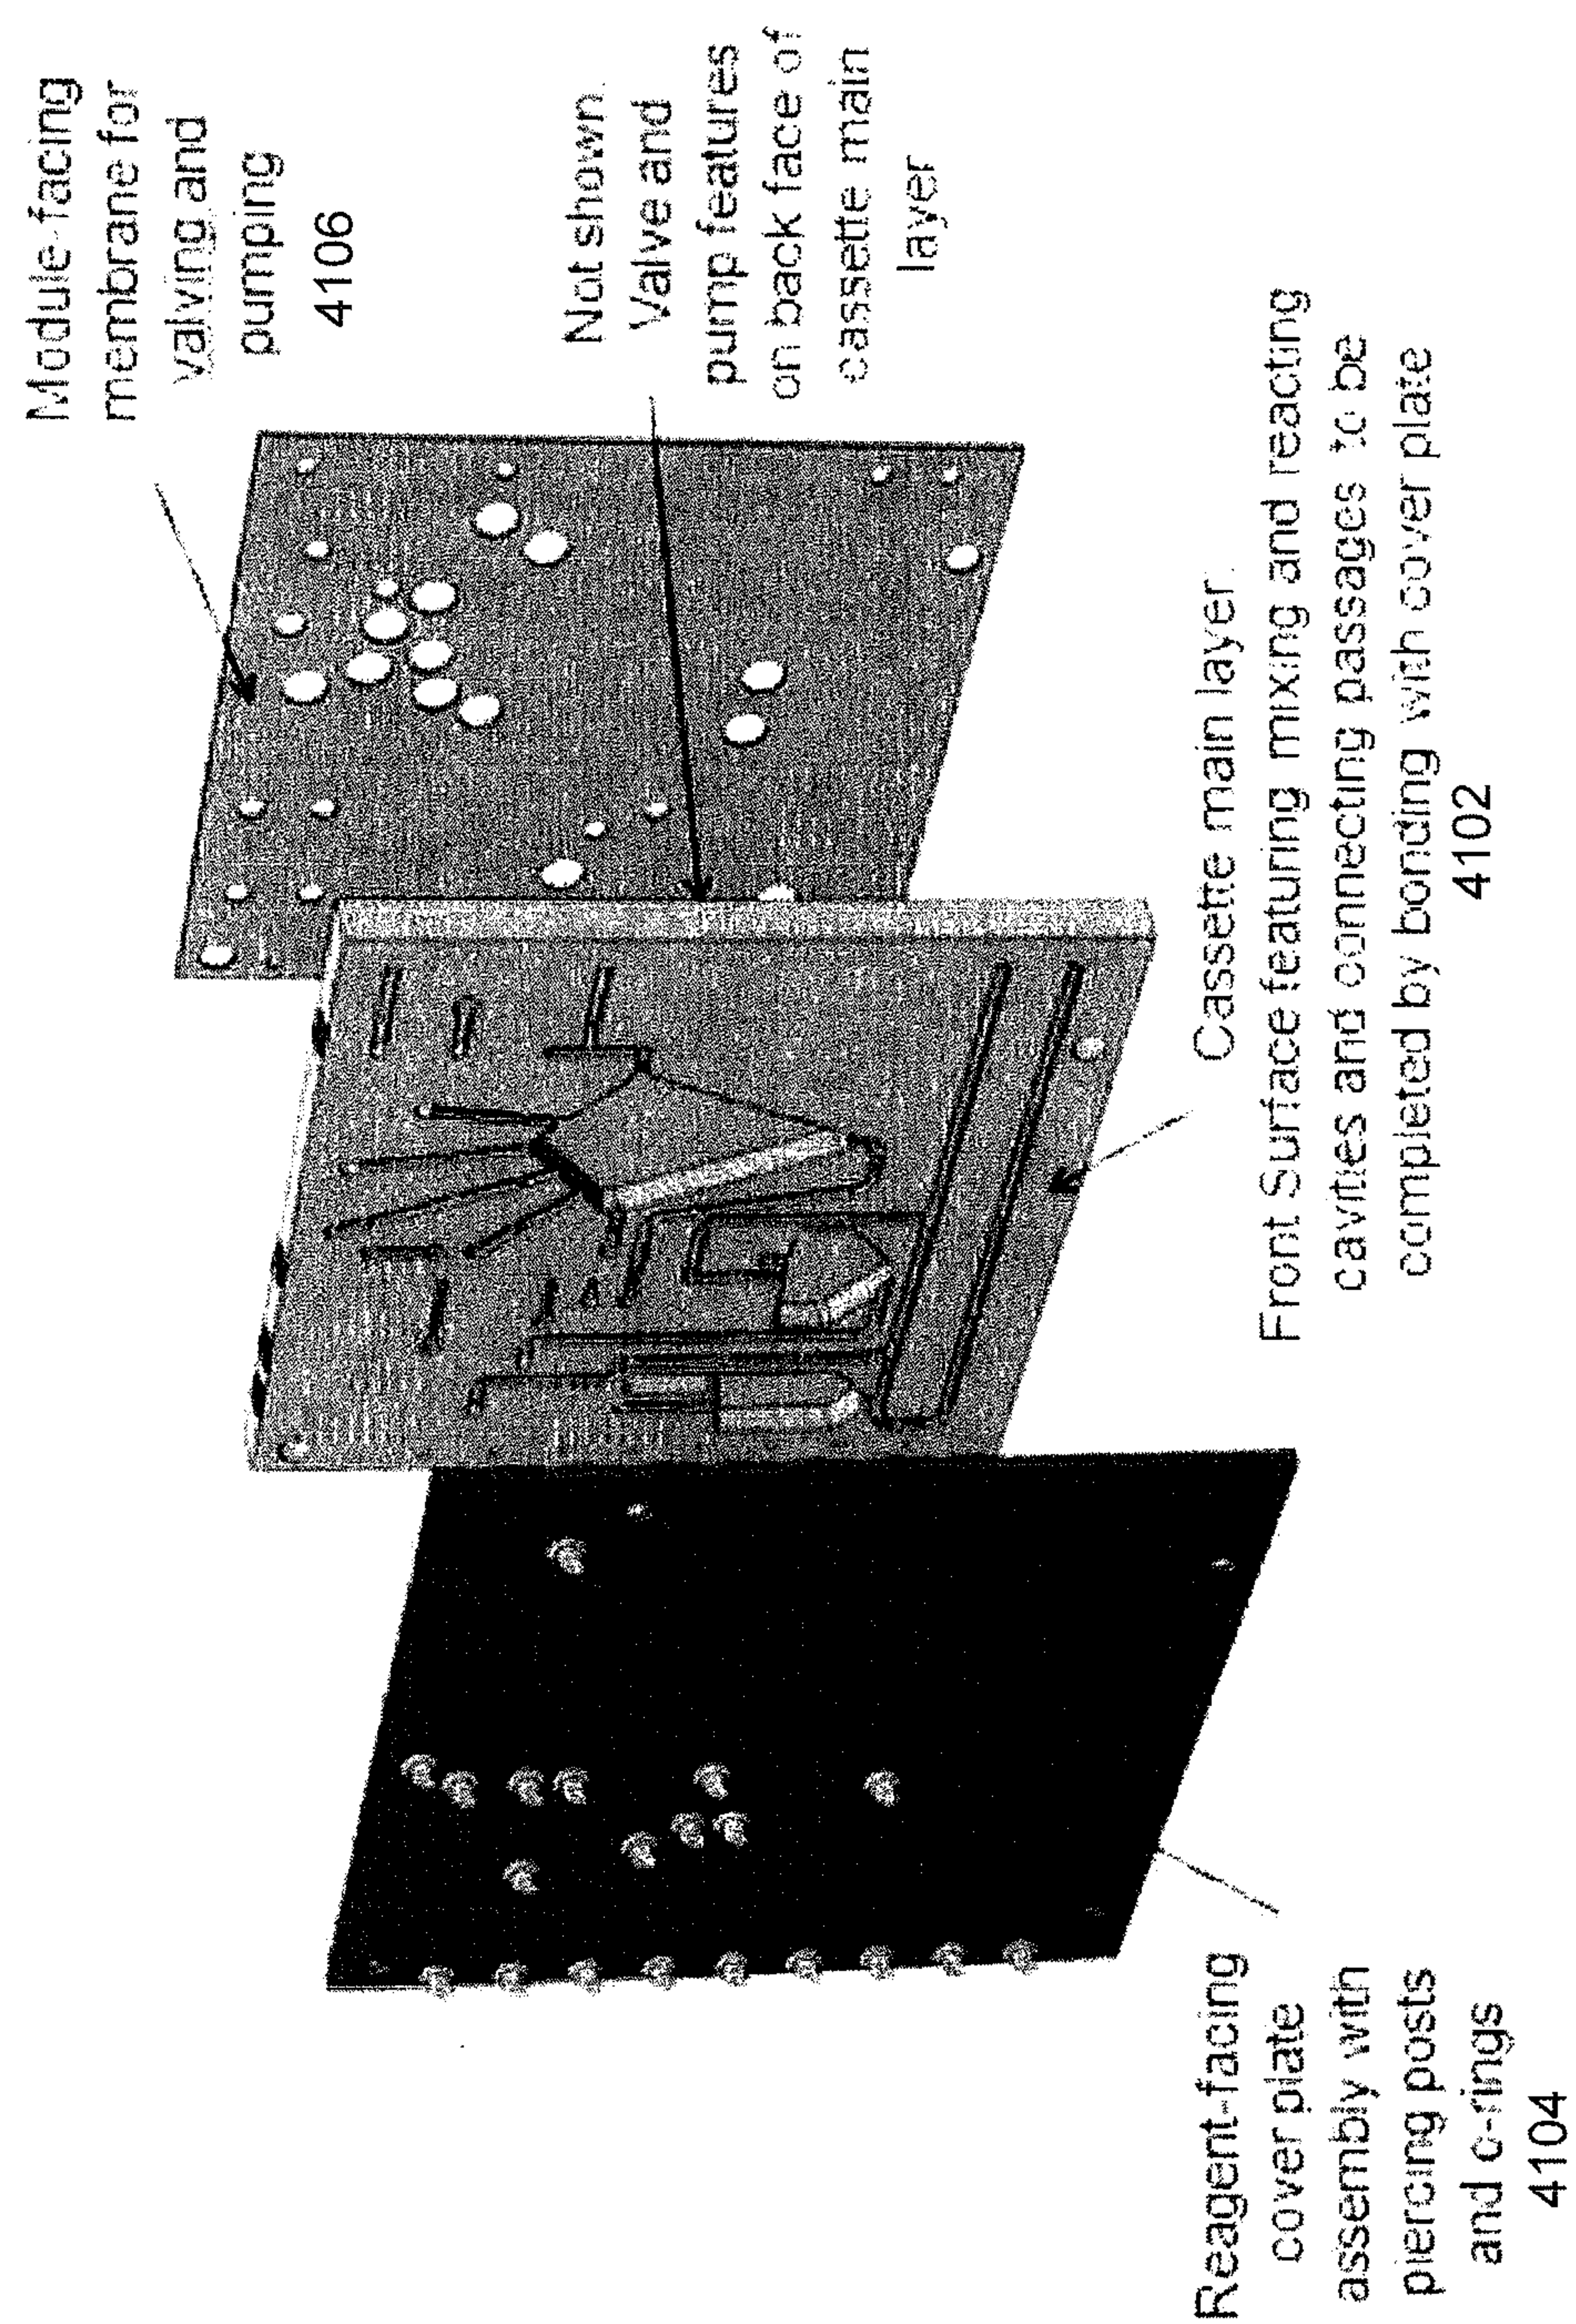


FIG. 41



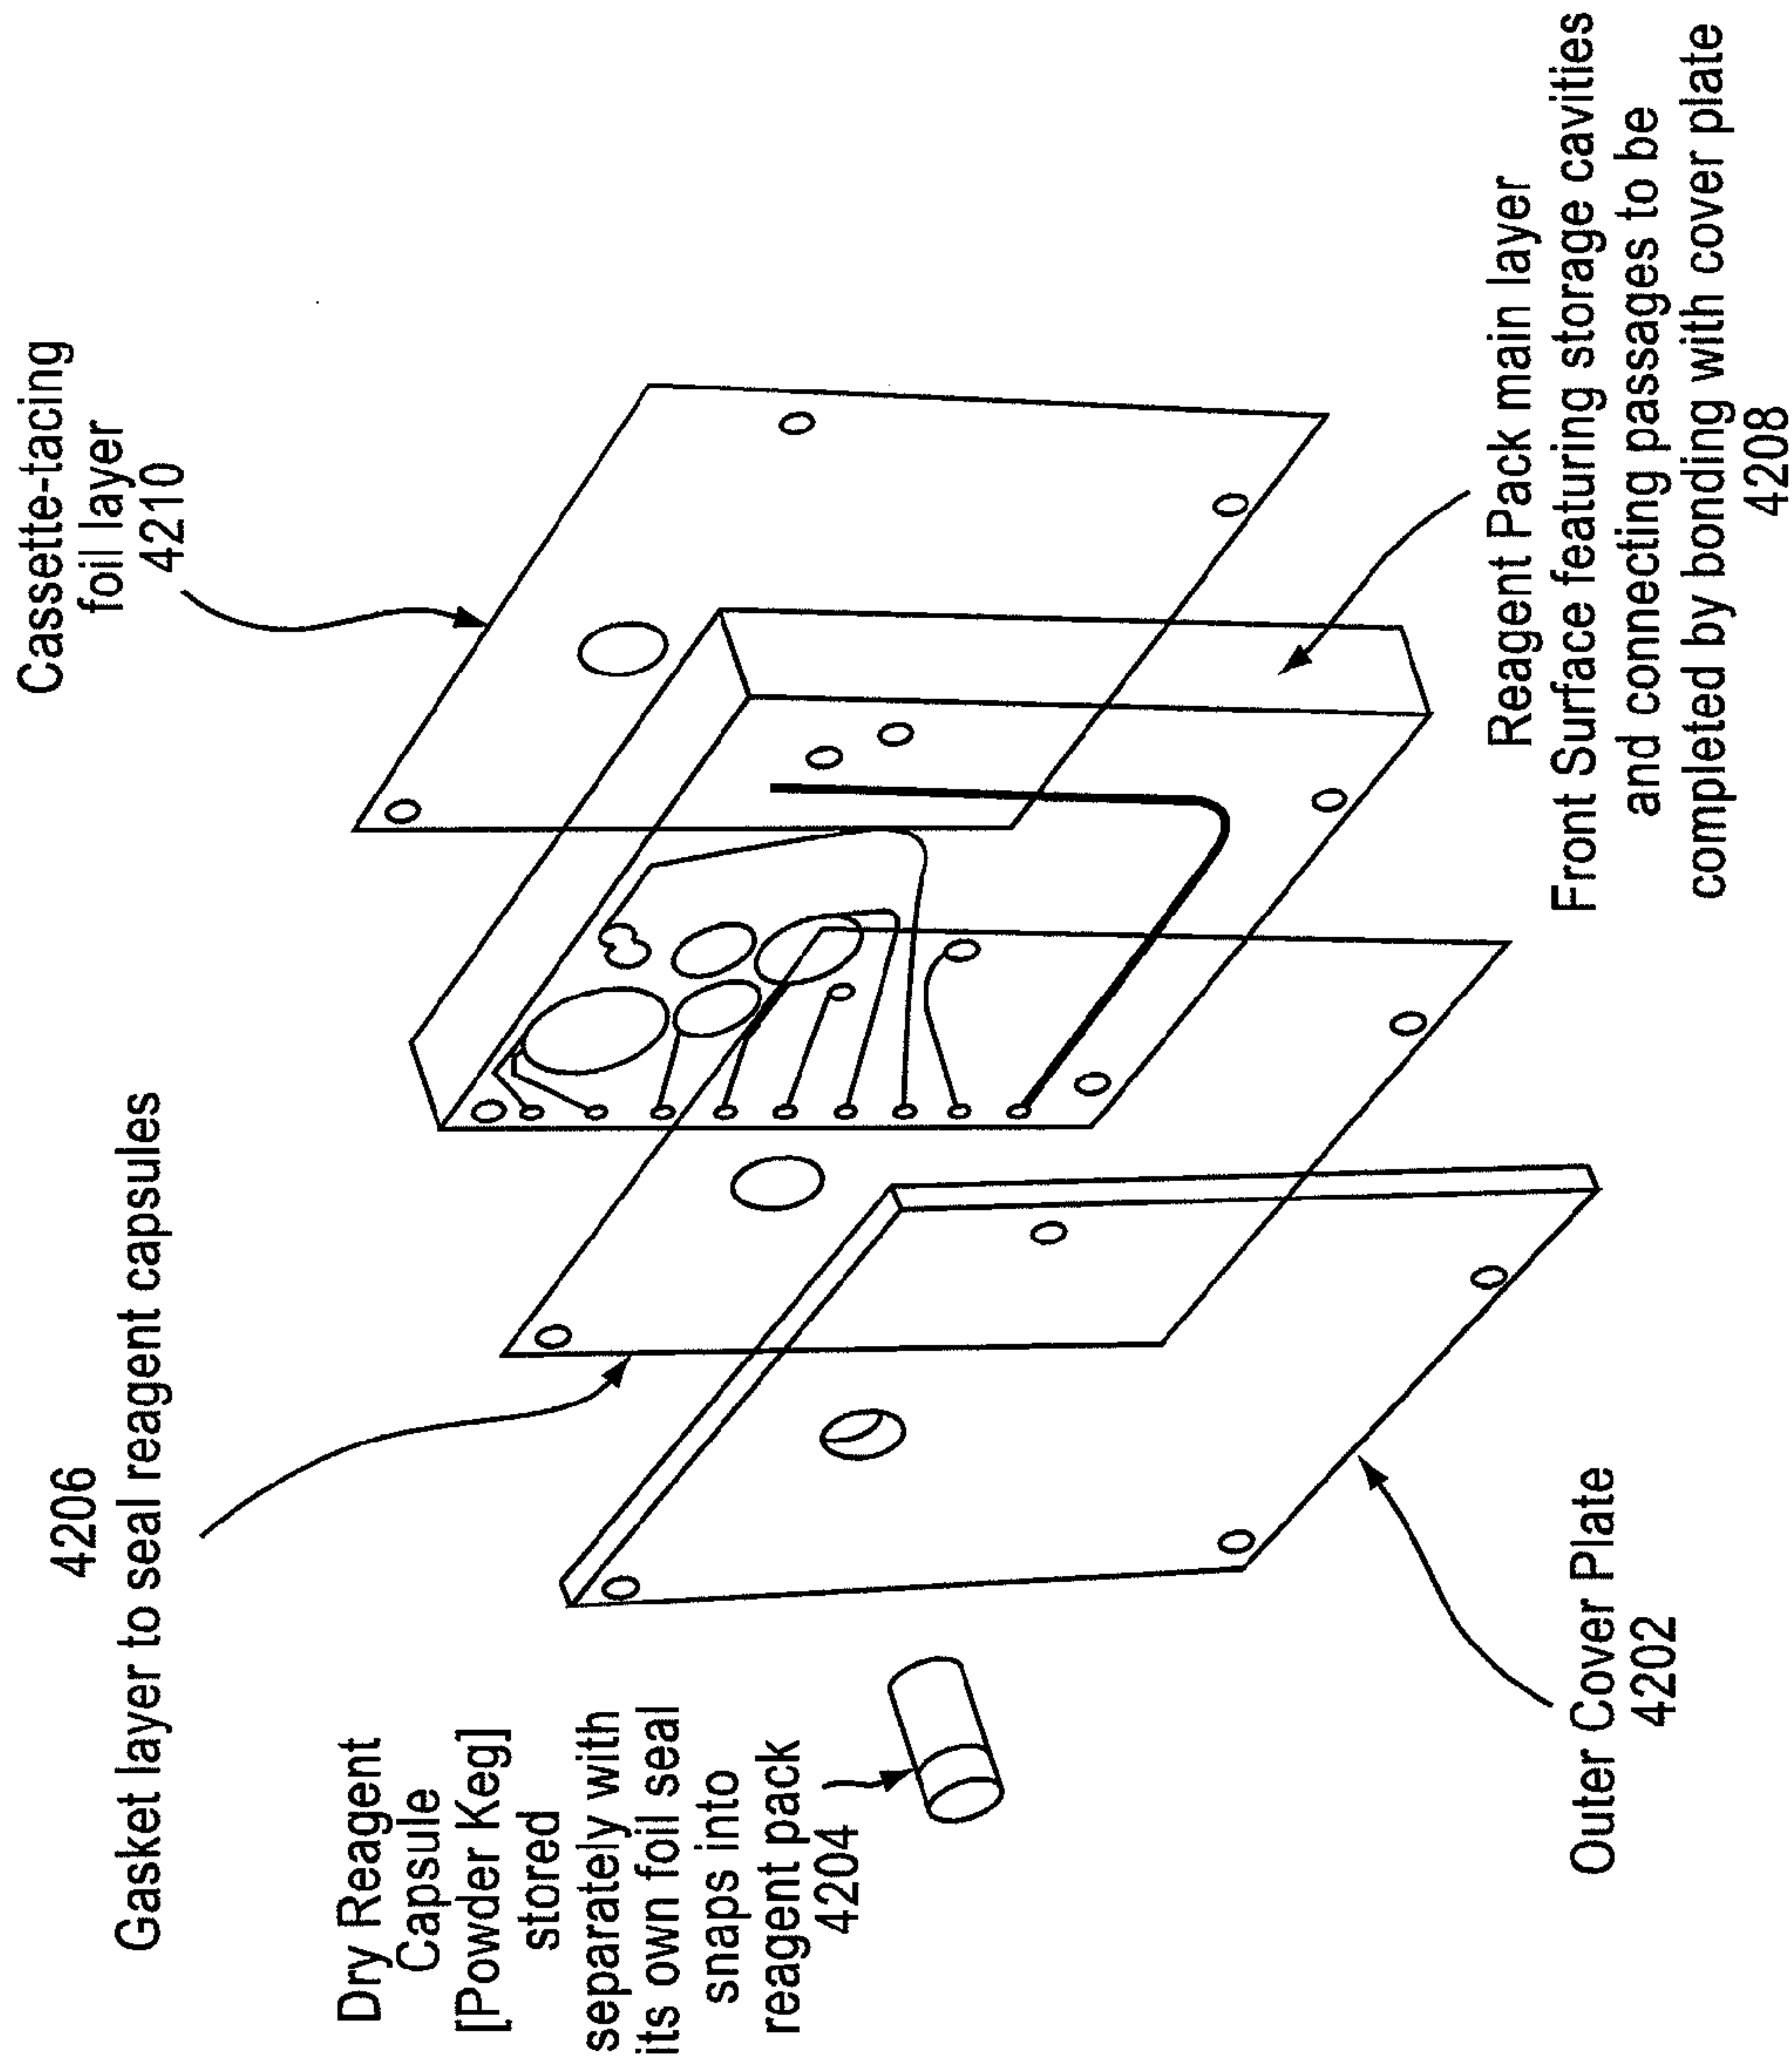


FIG.42



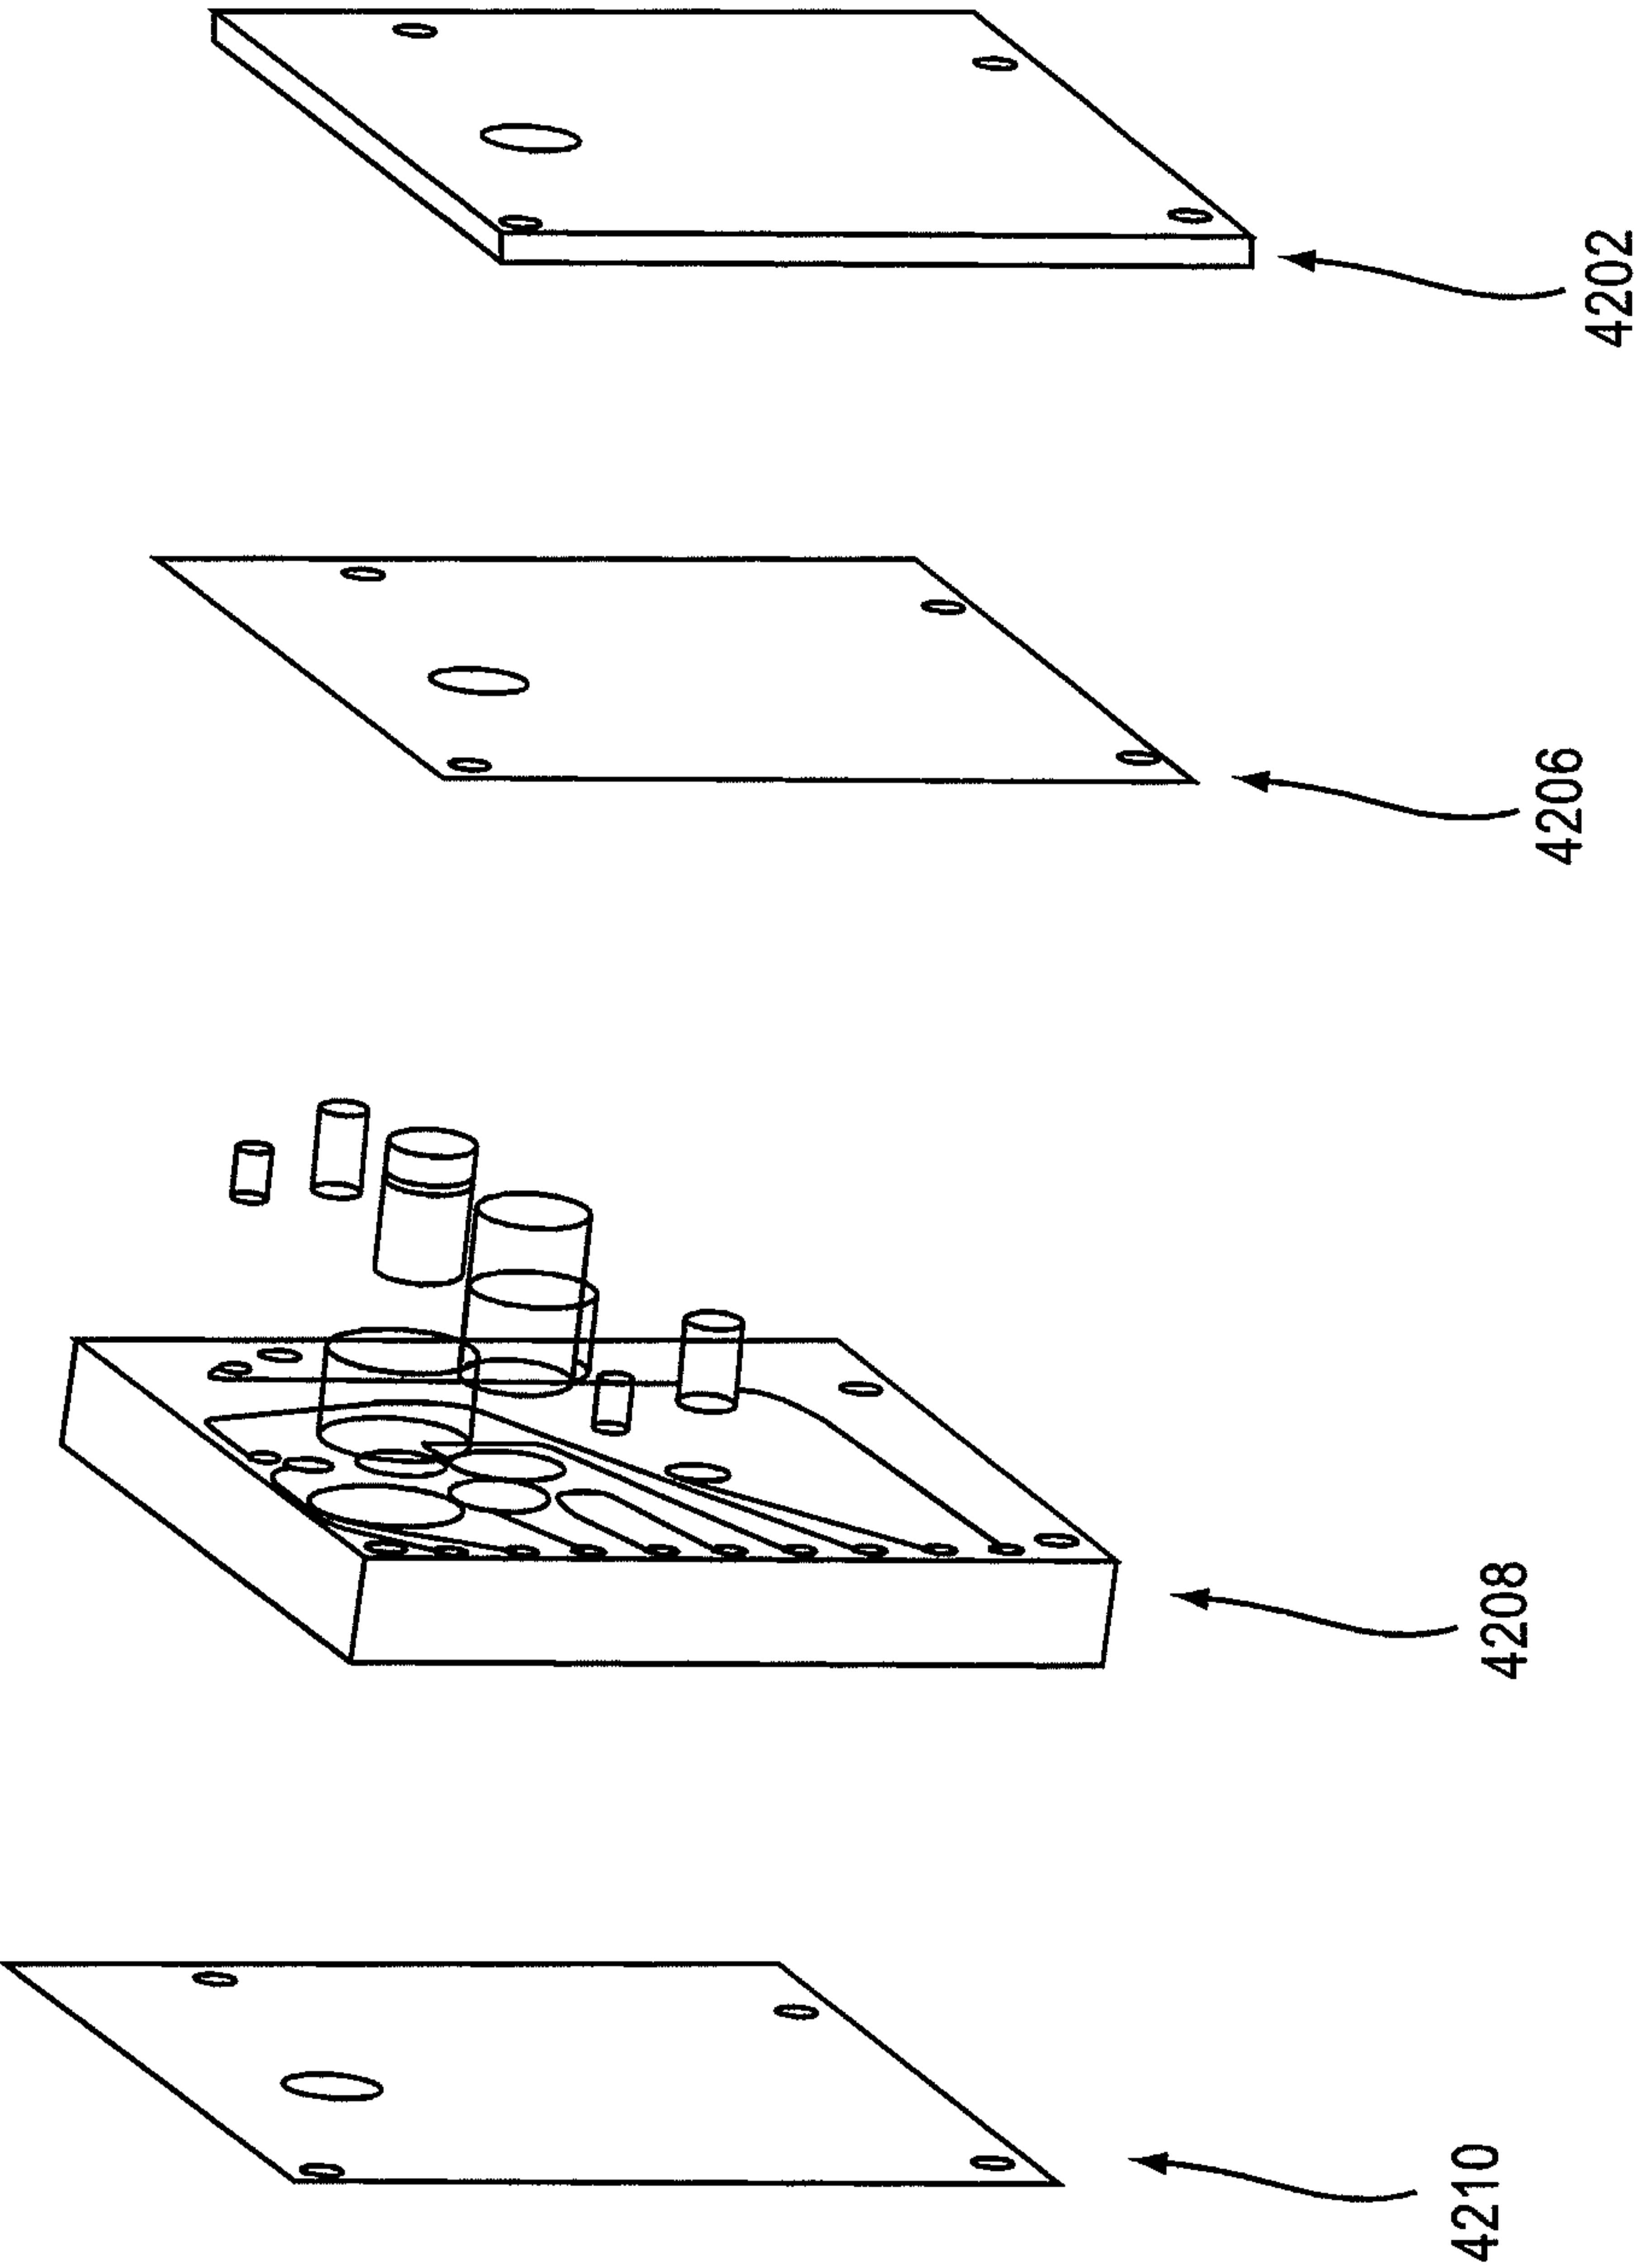


FIG.43



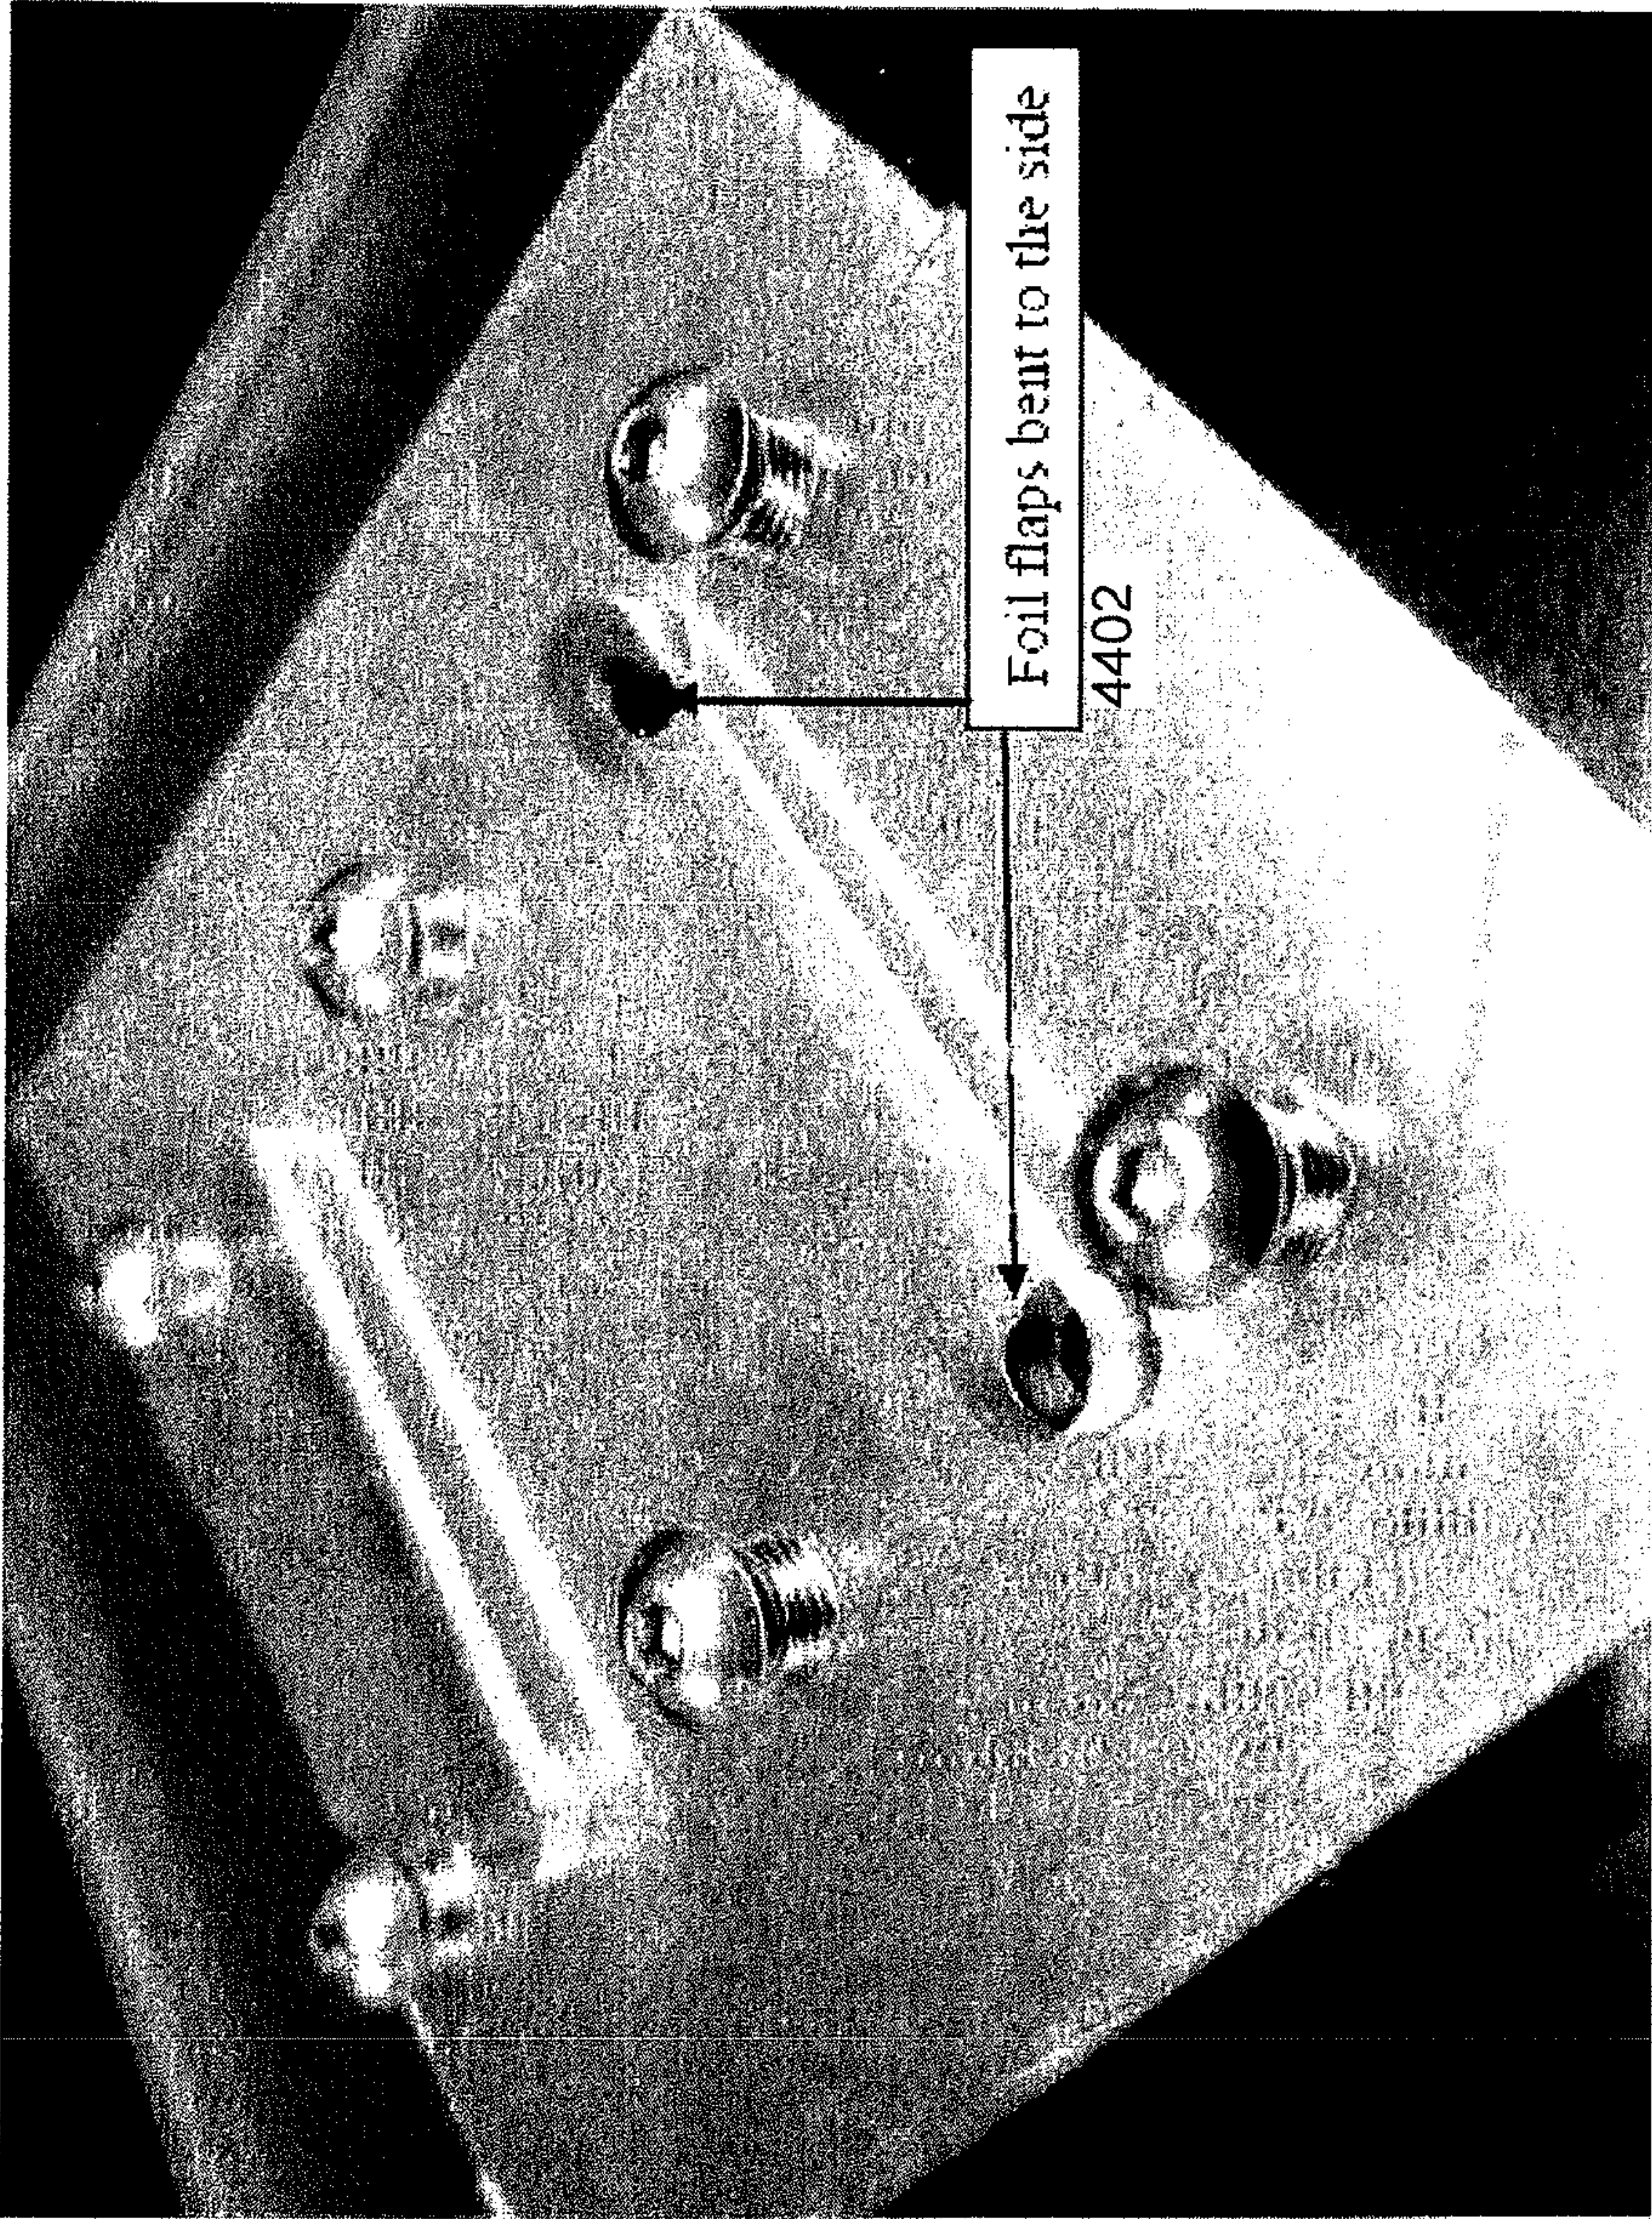


FIG. 44



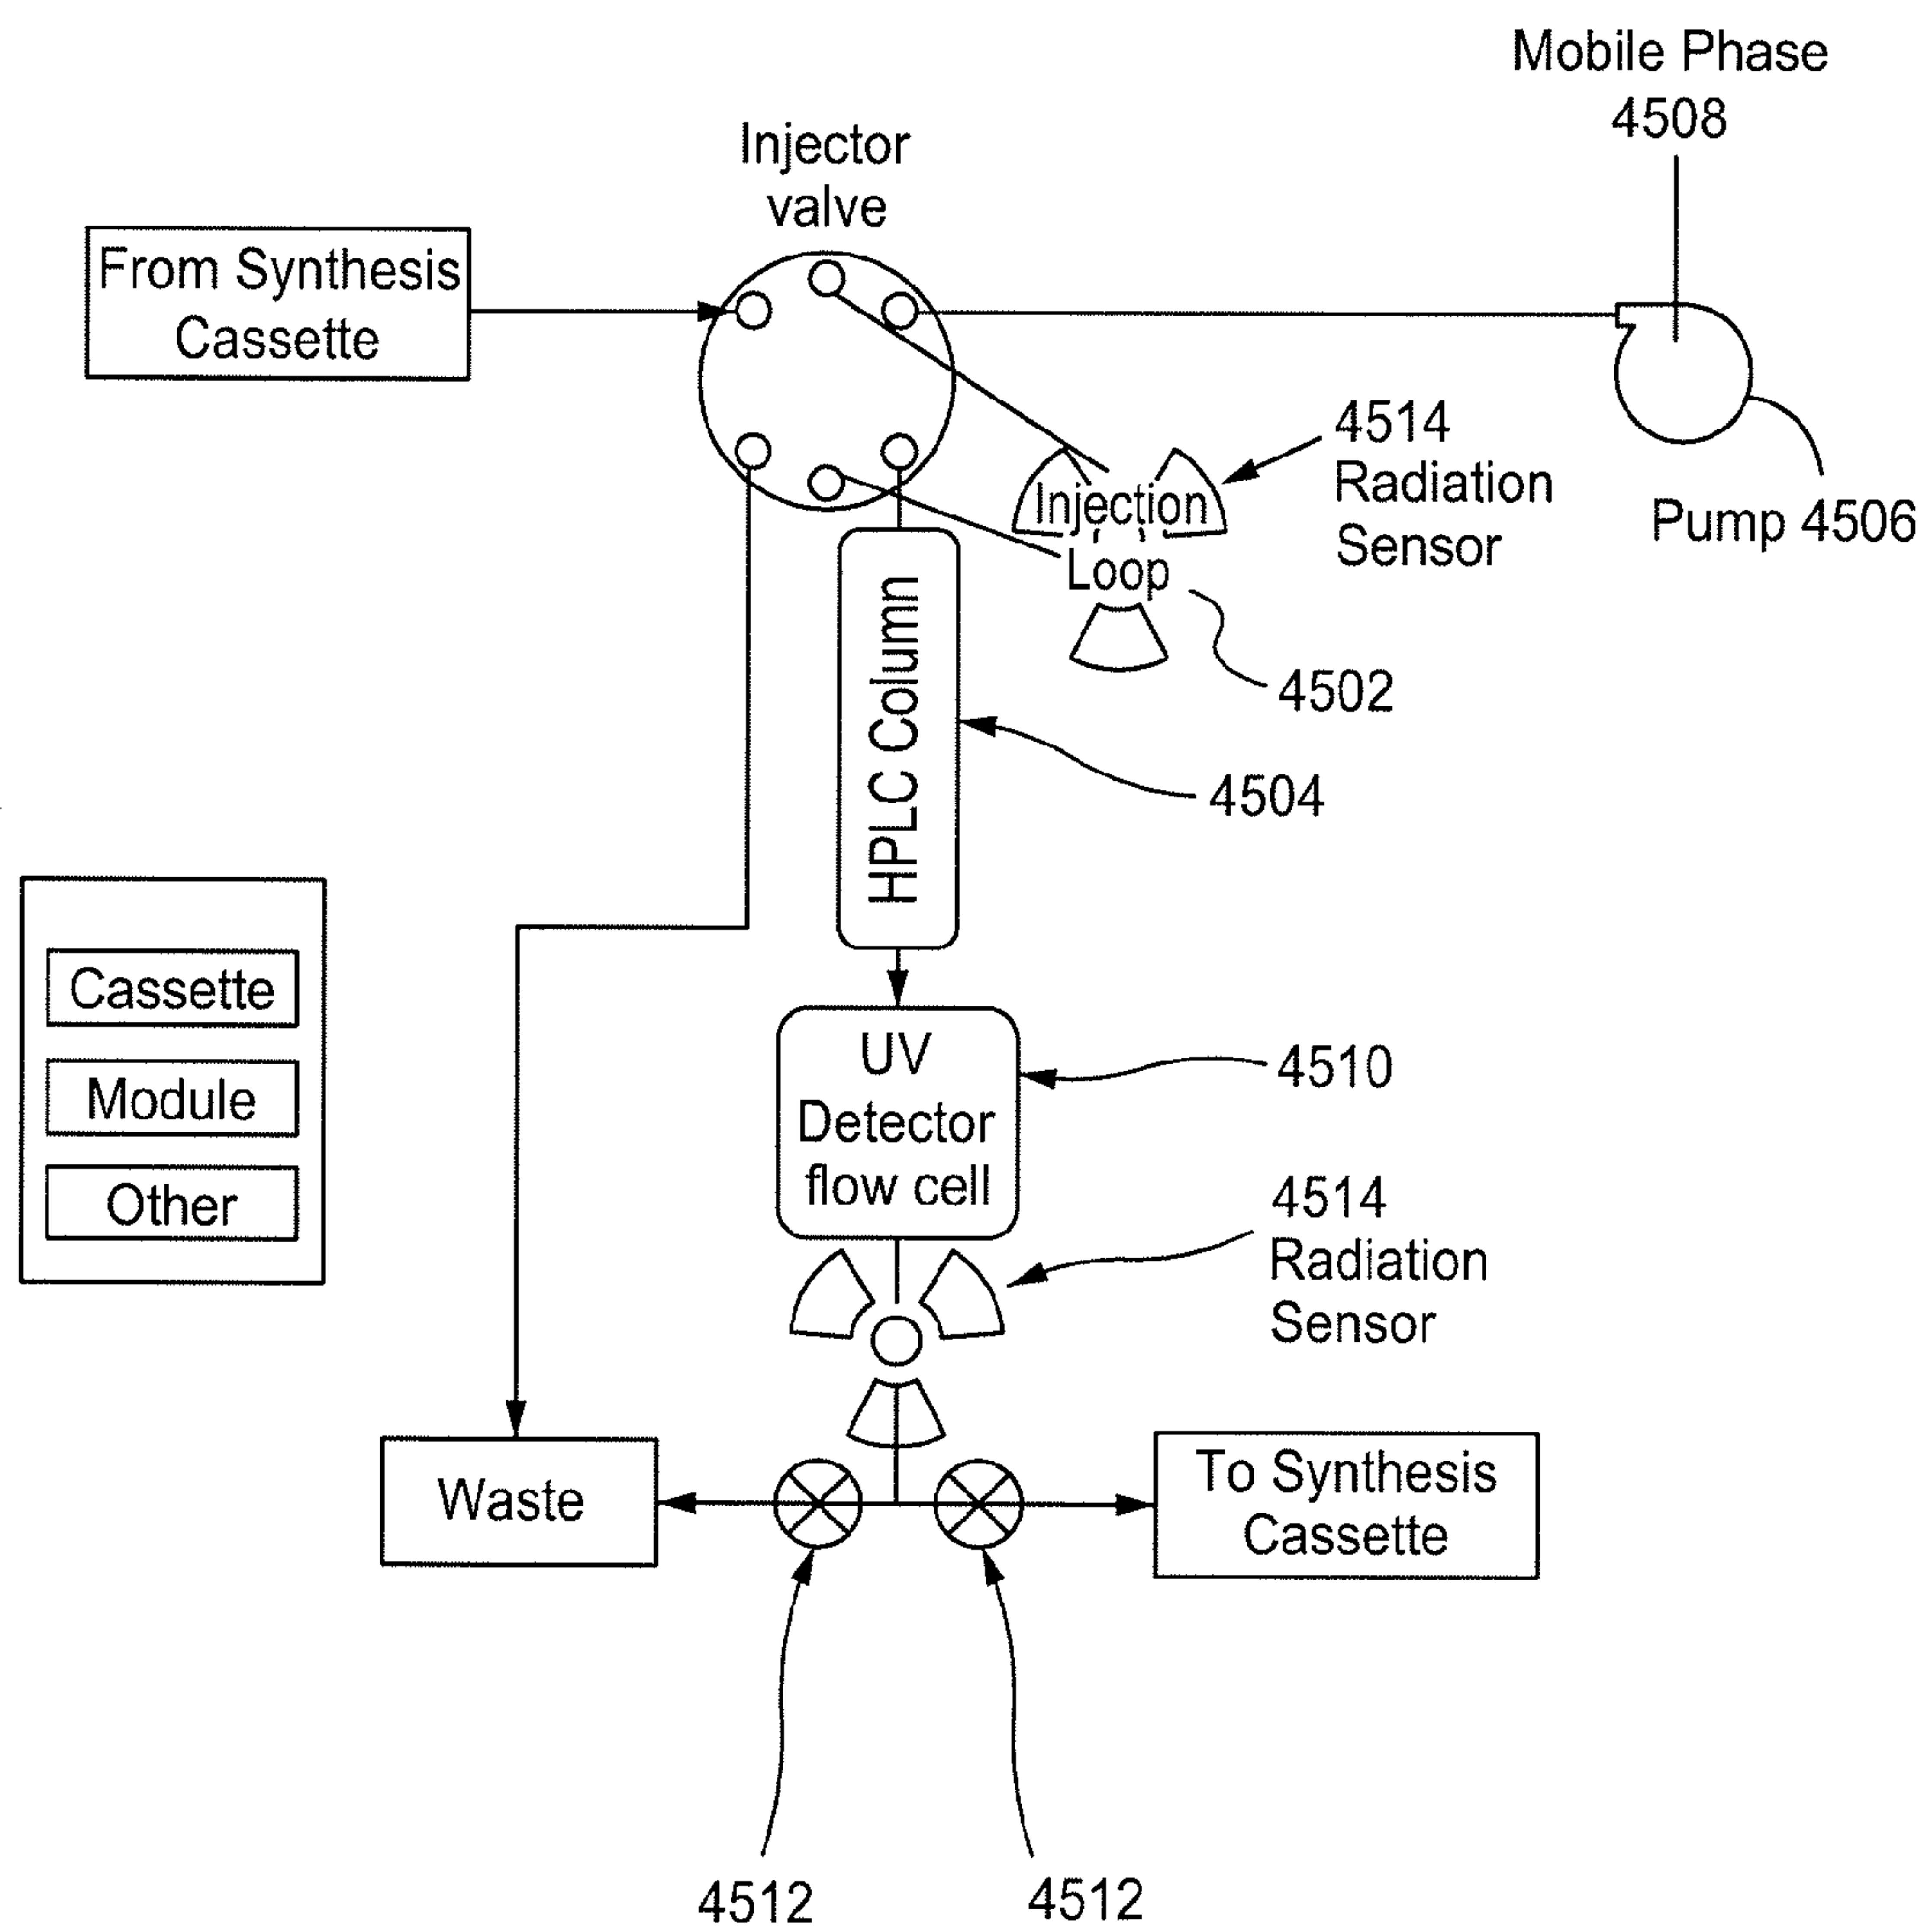


Fig.45

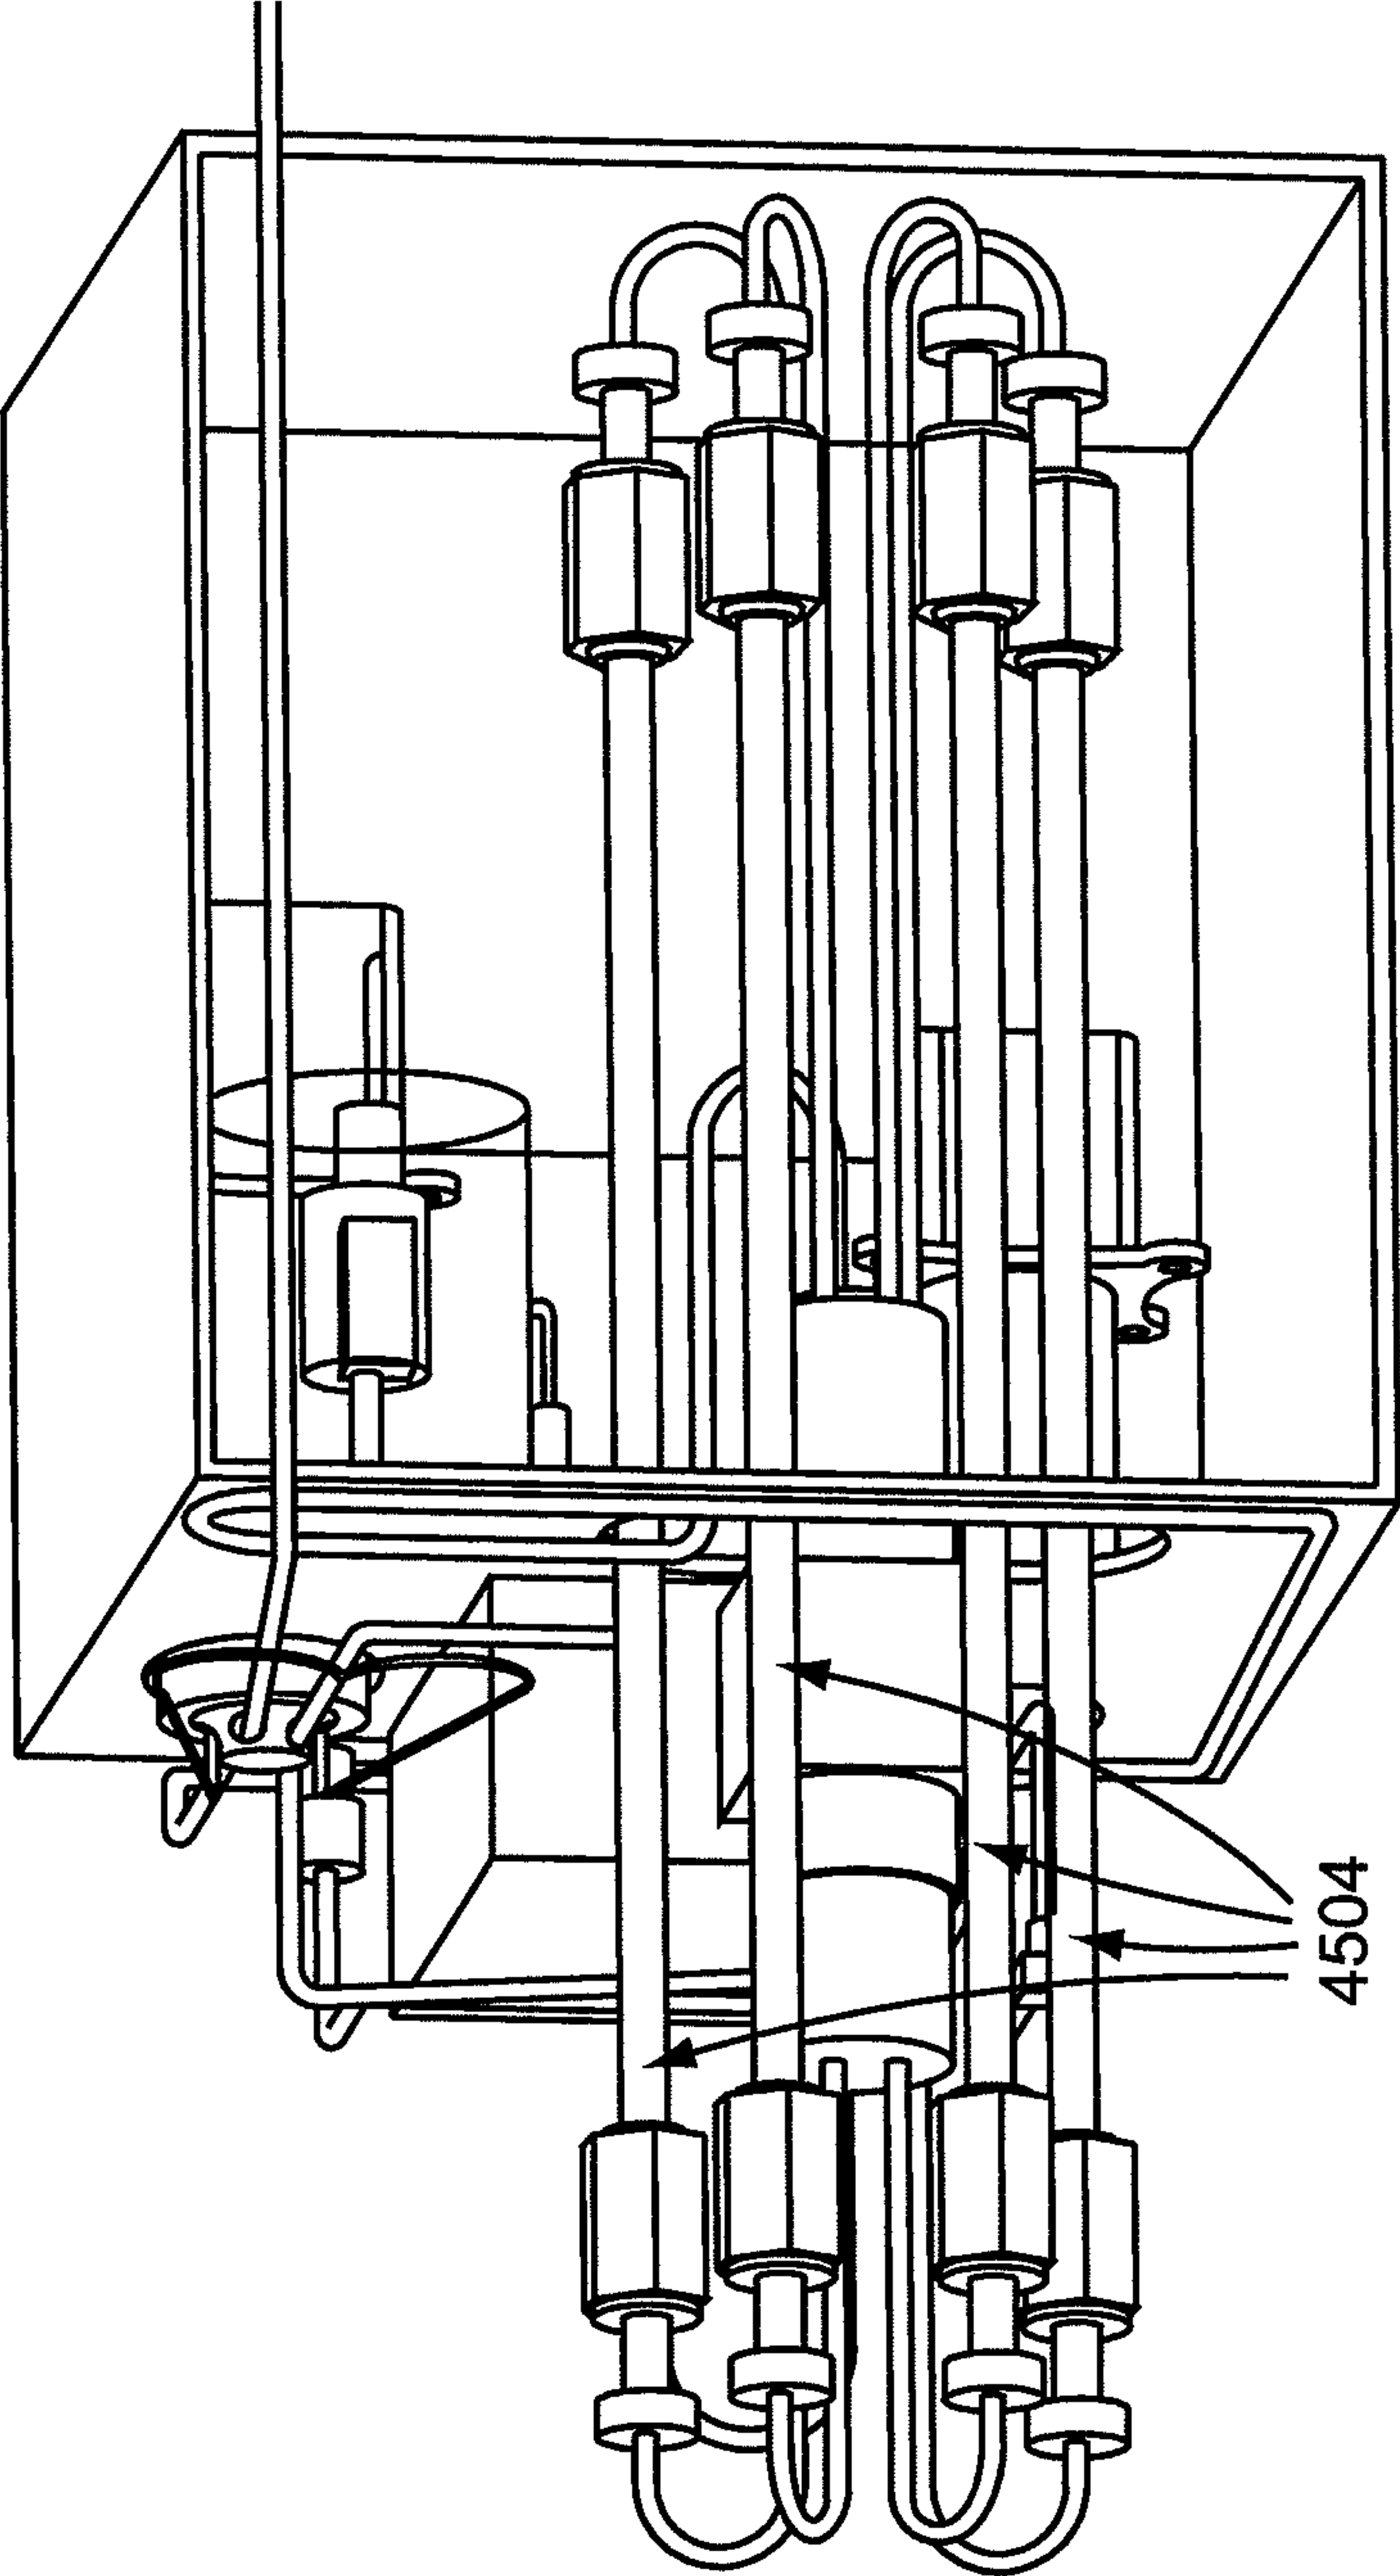


Fig. 46



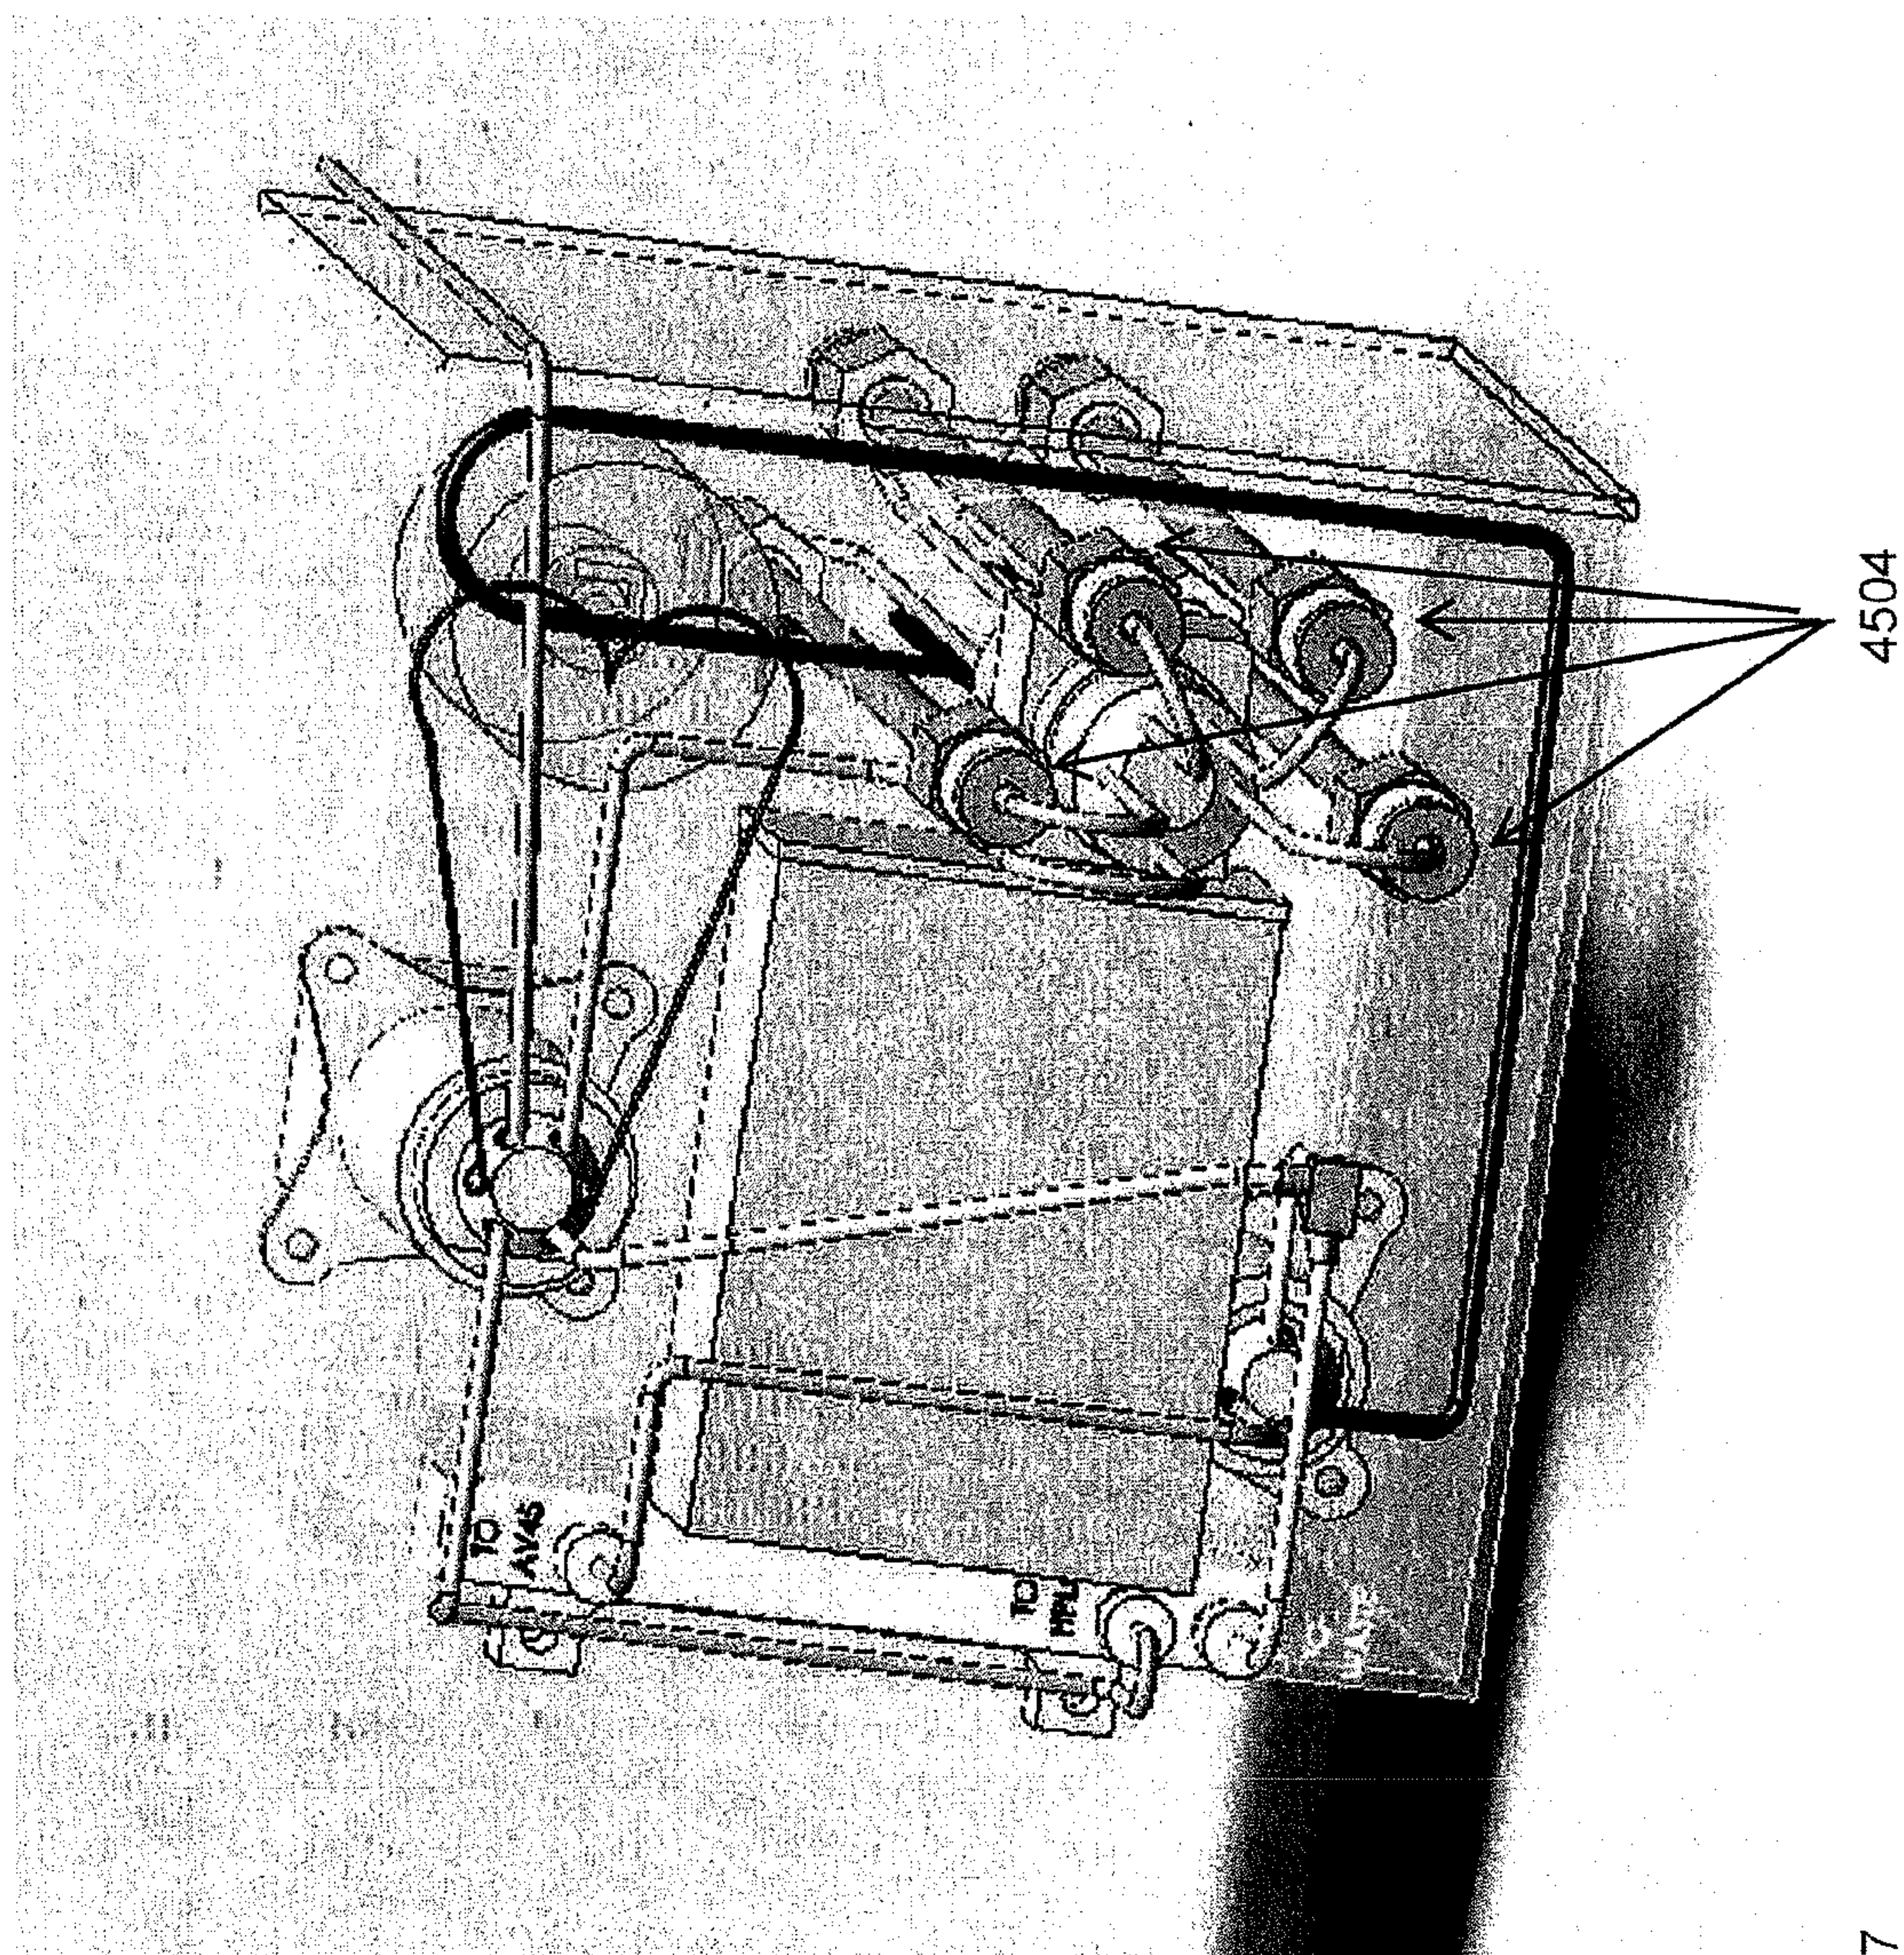
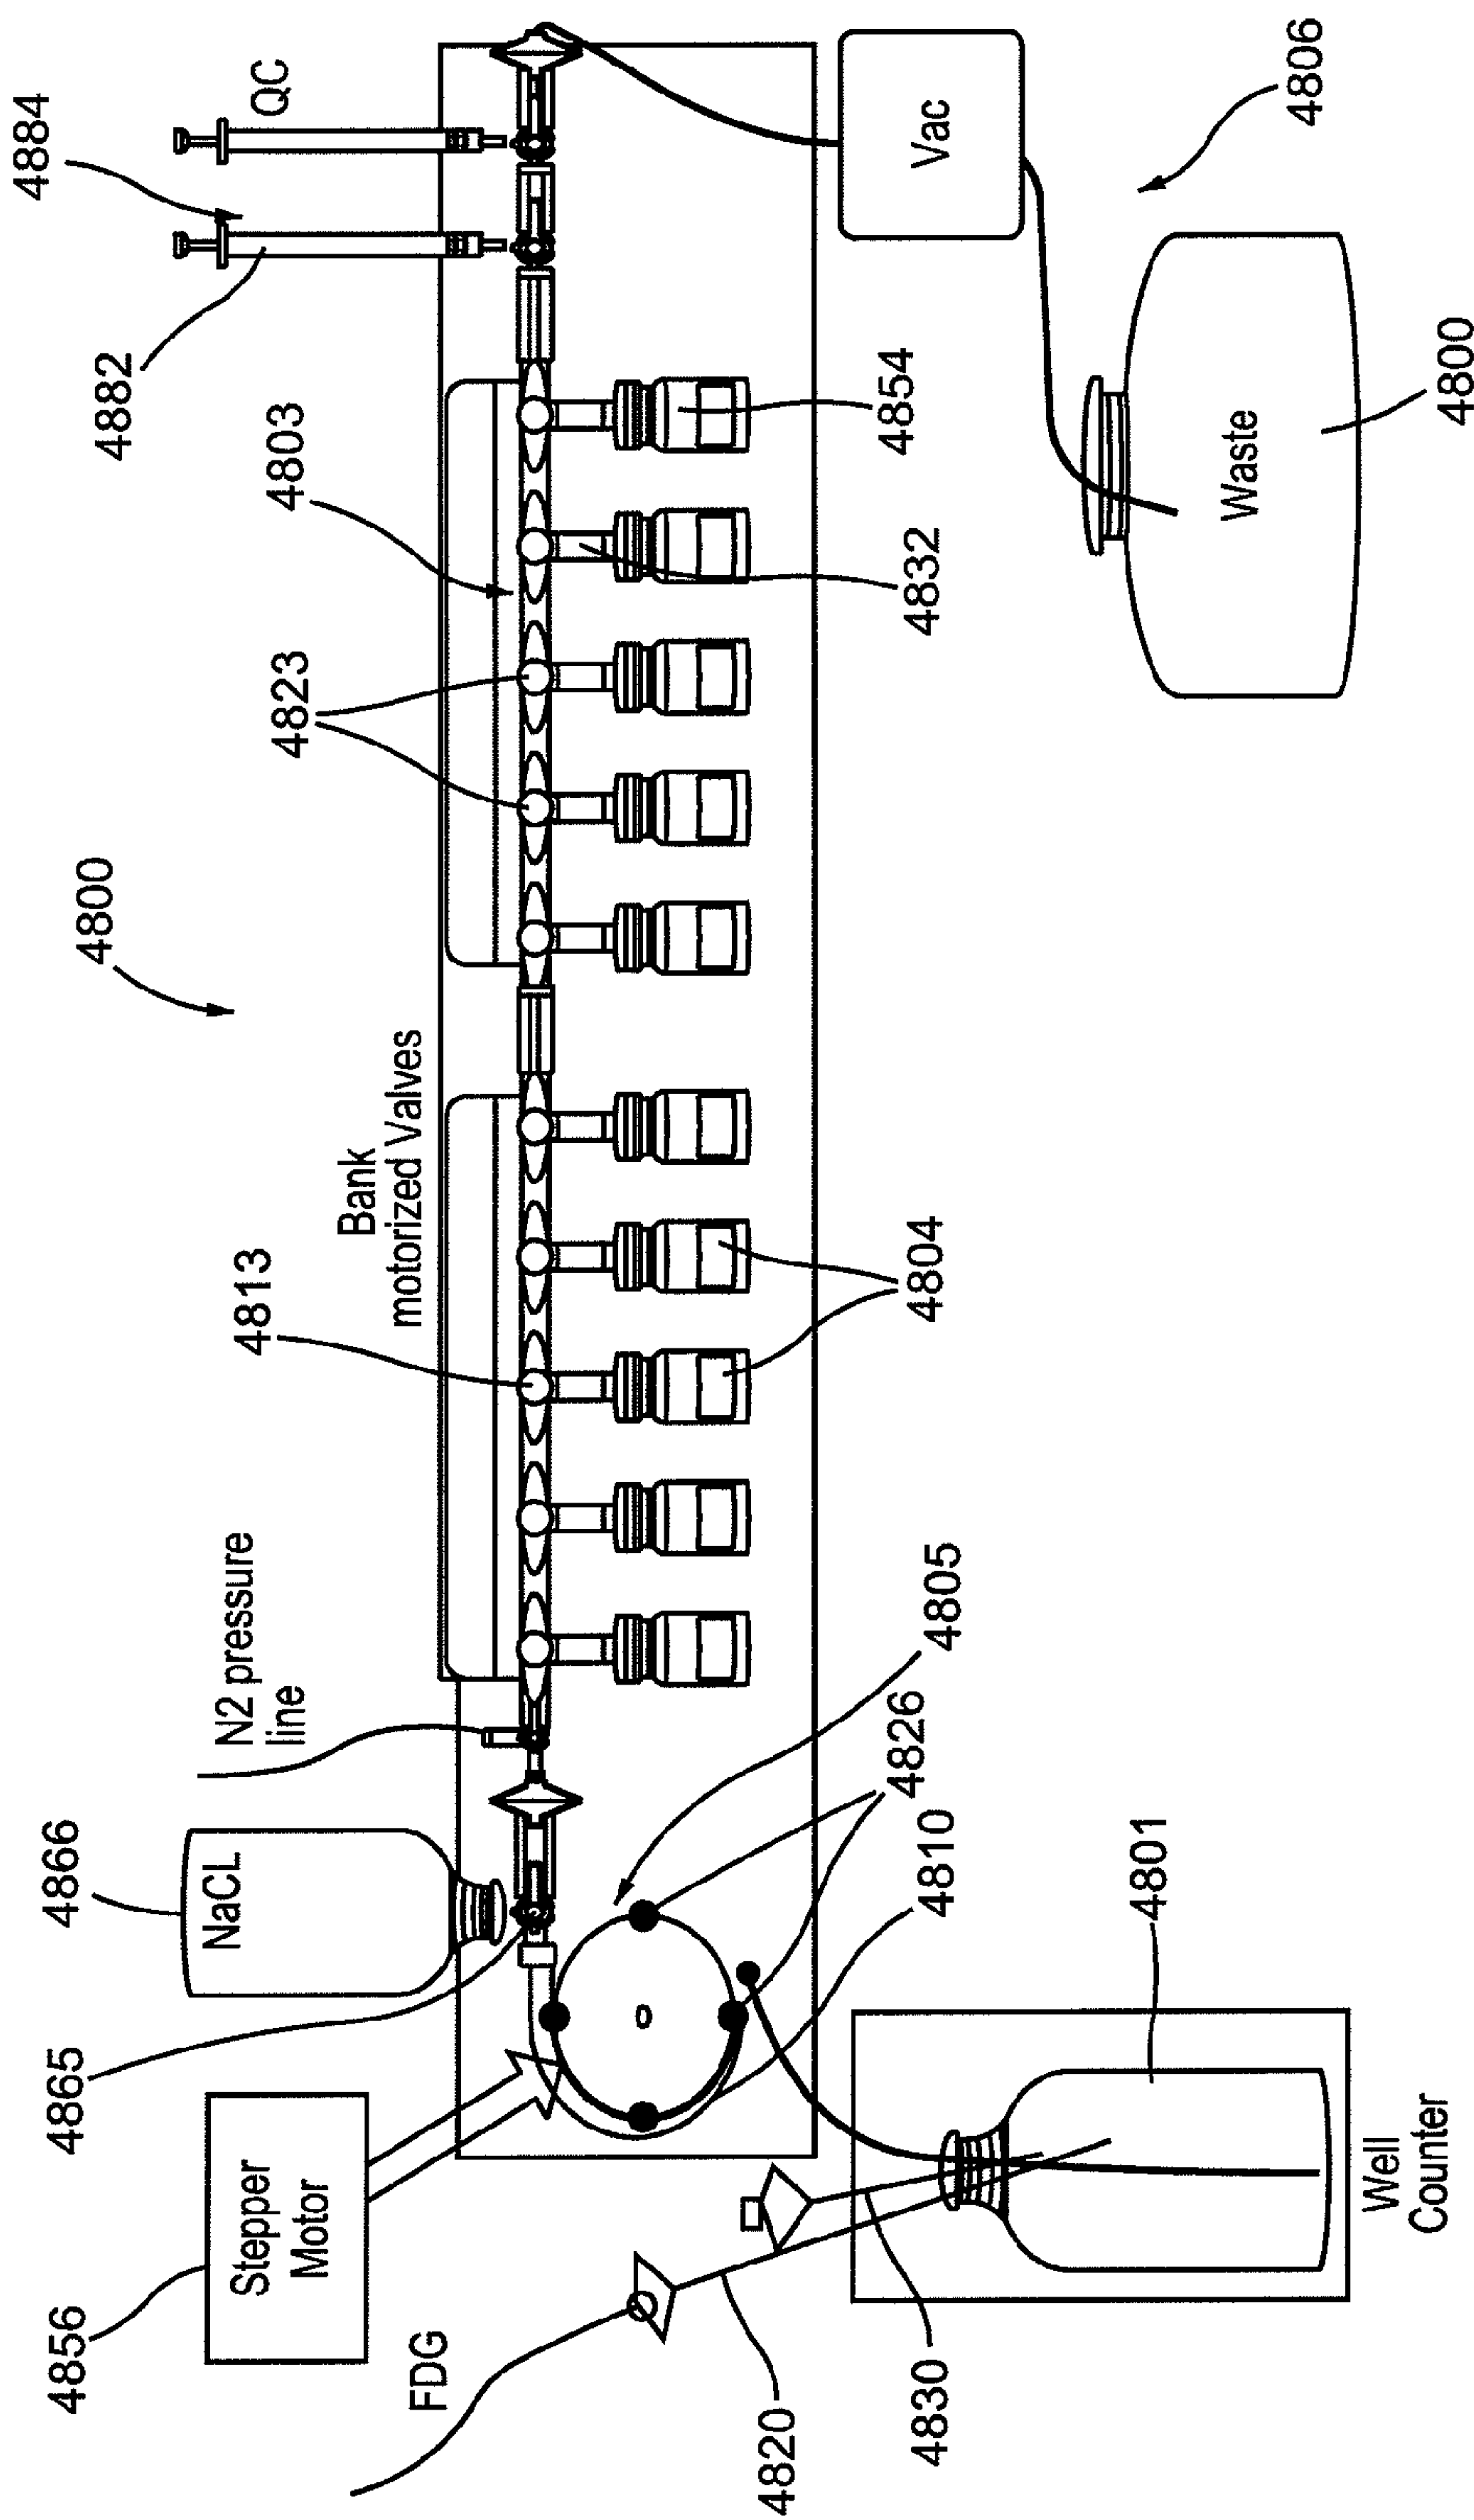


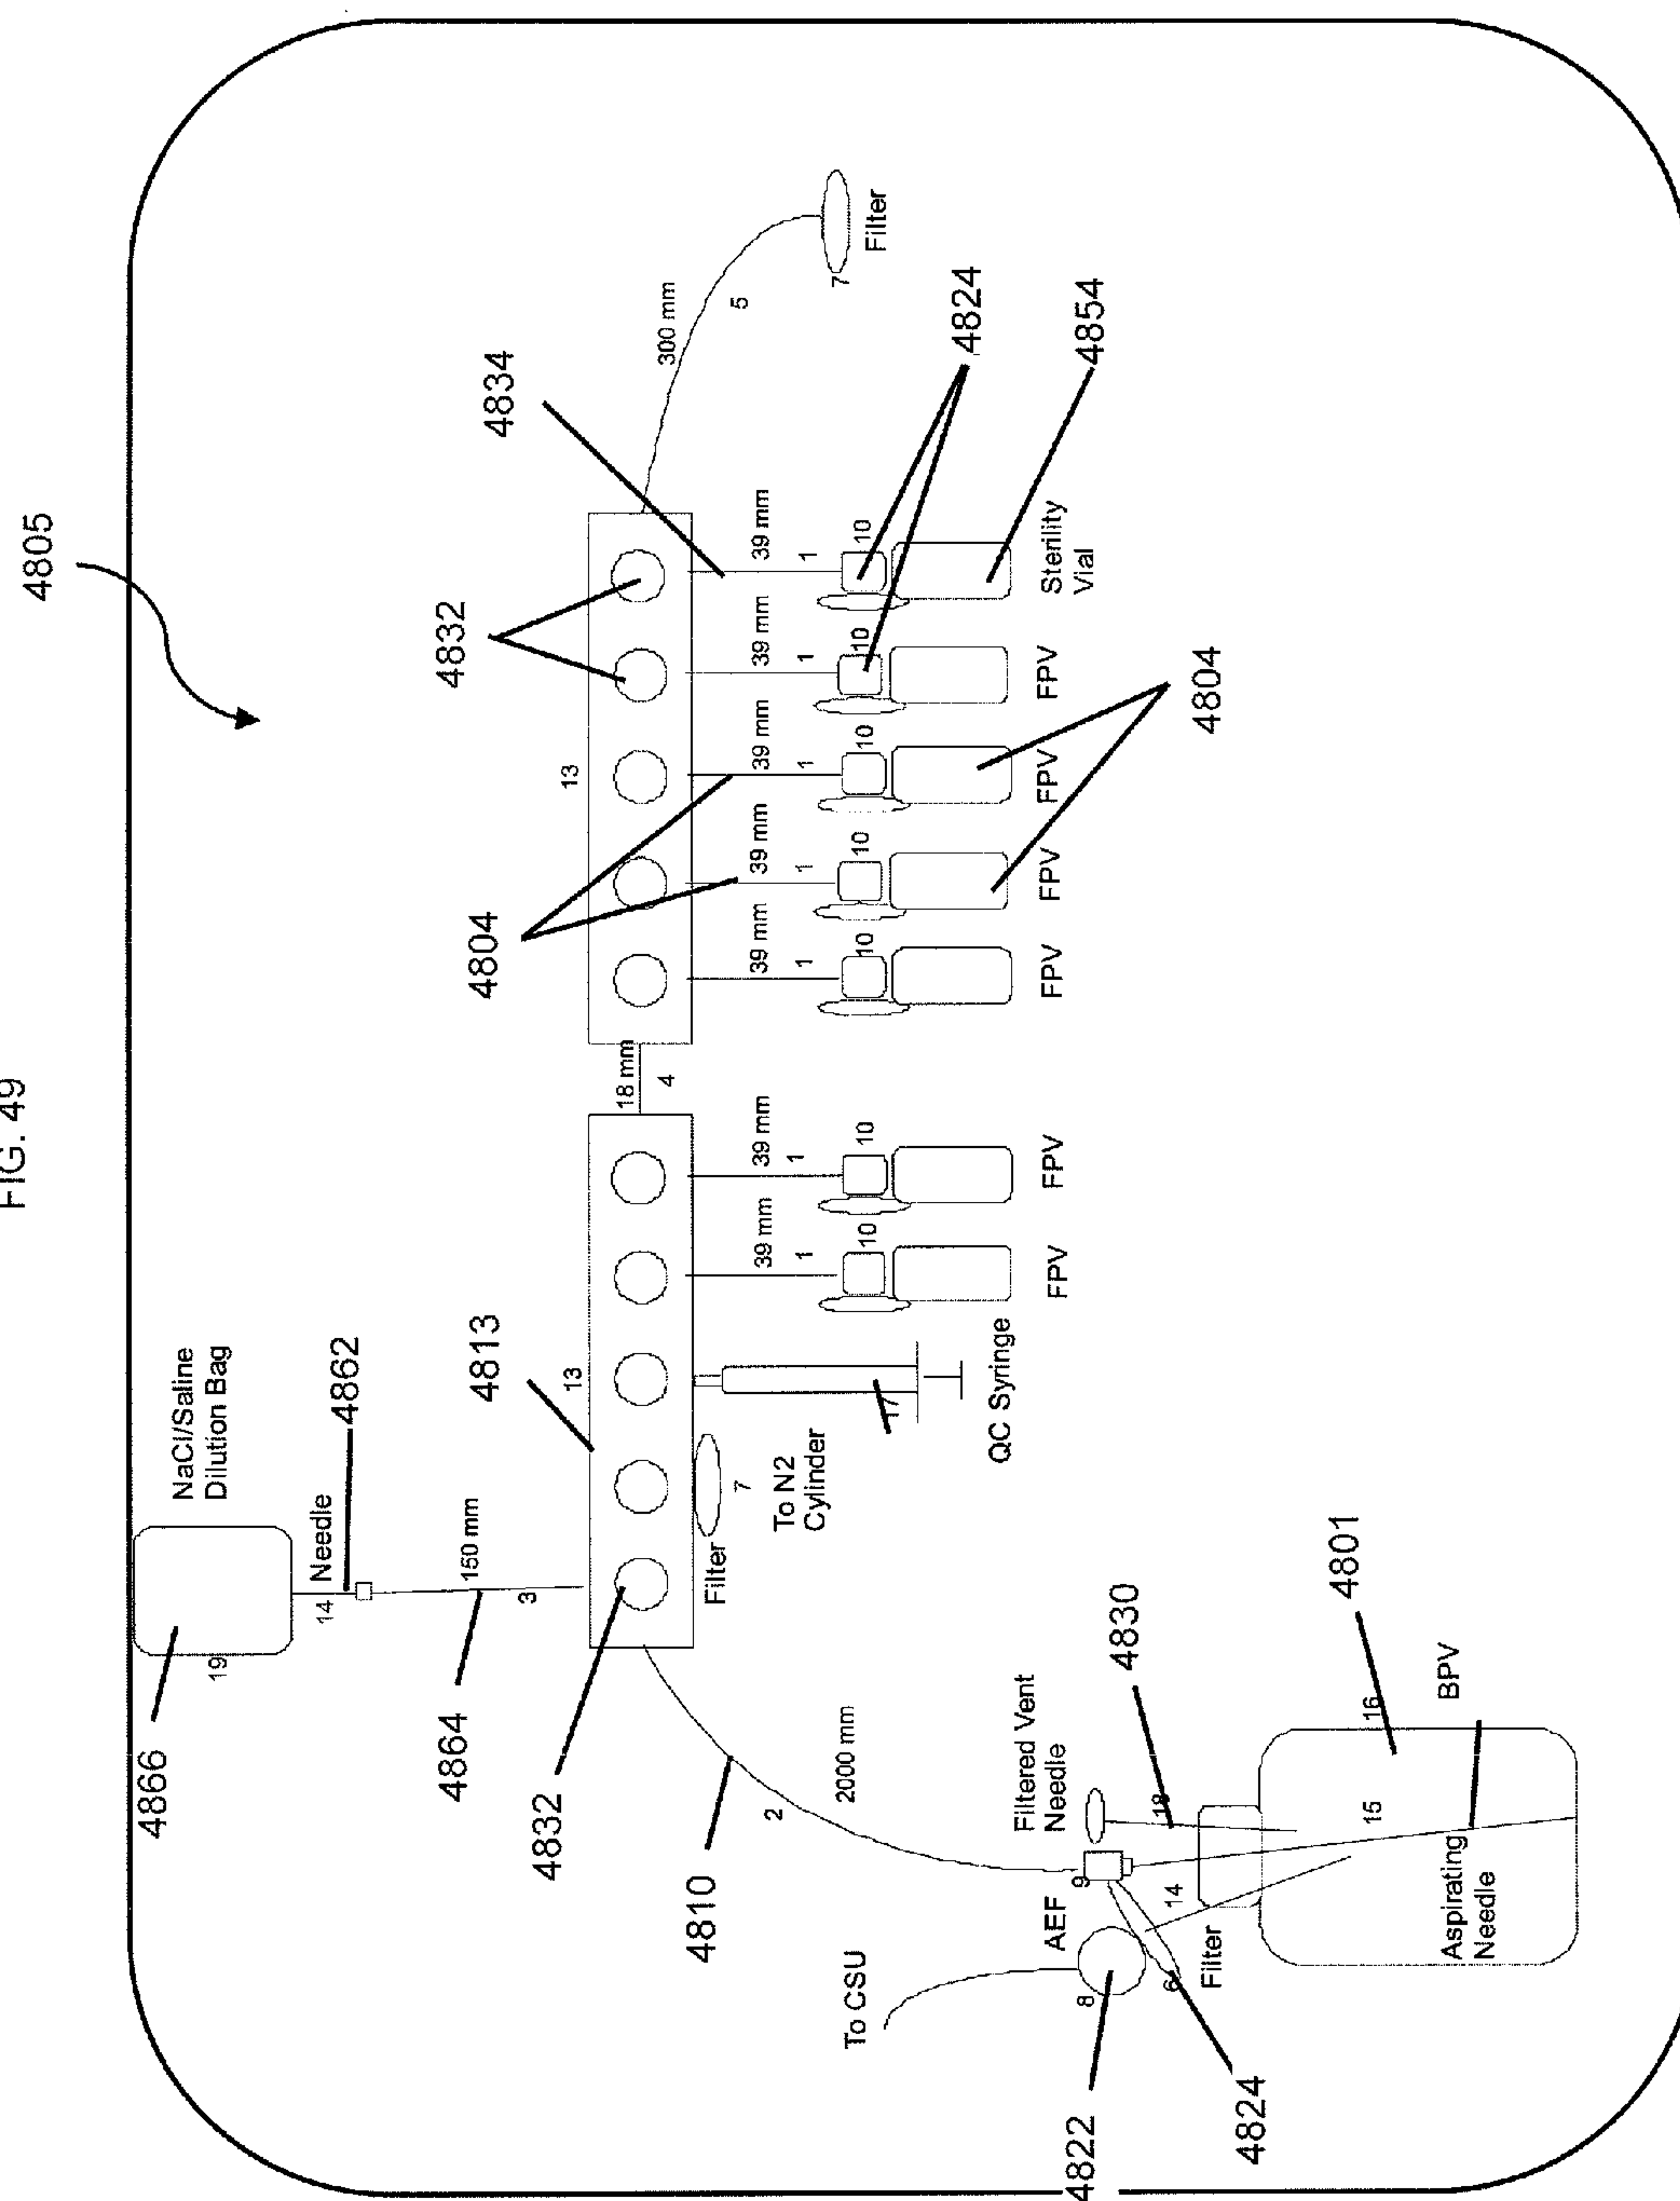



FIG. 48





F.G. 49



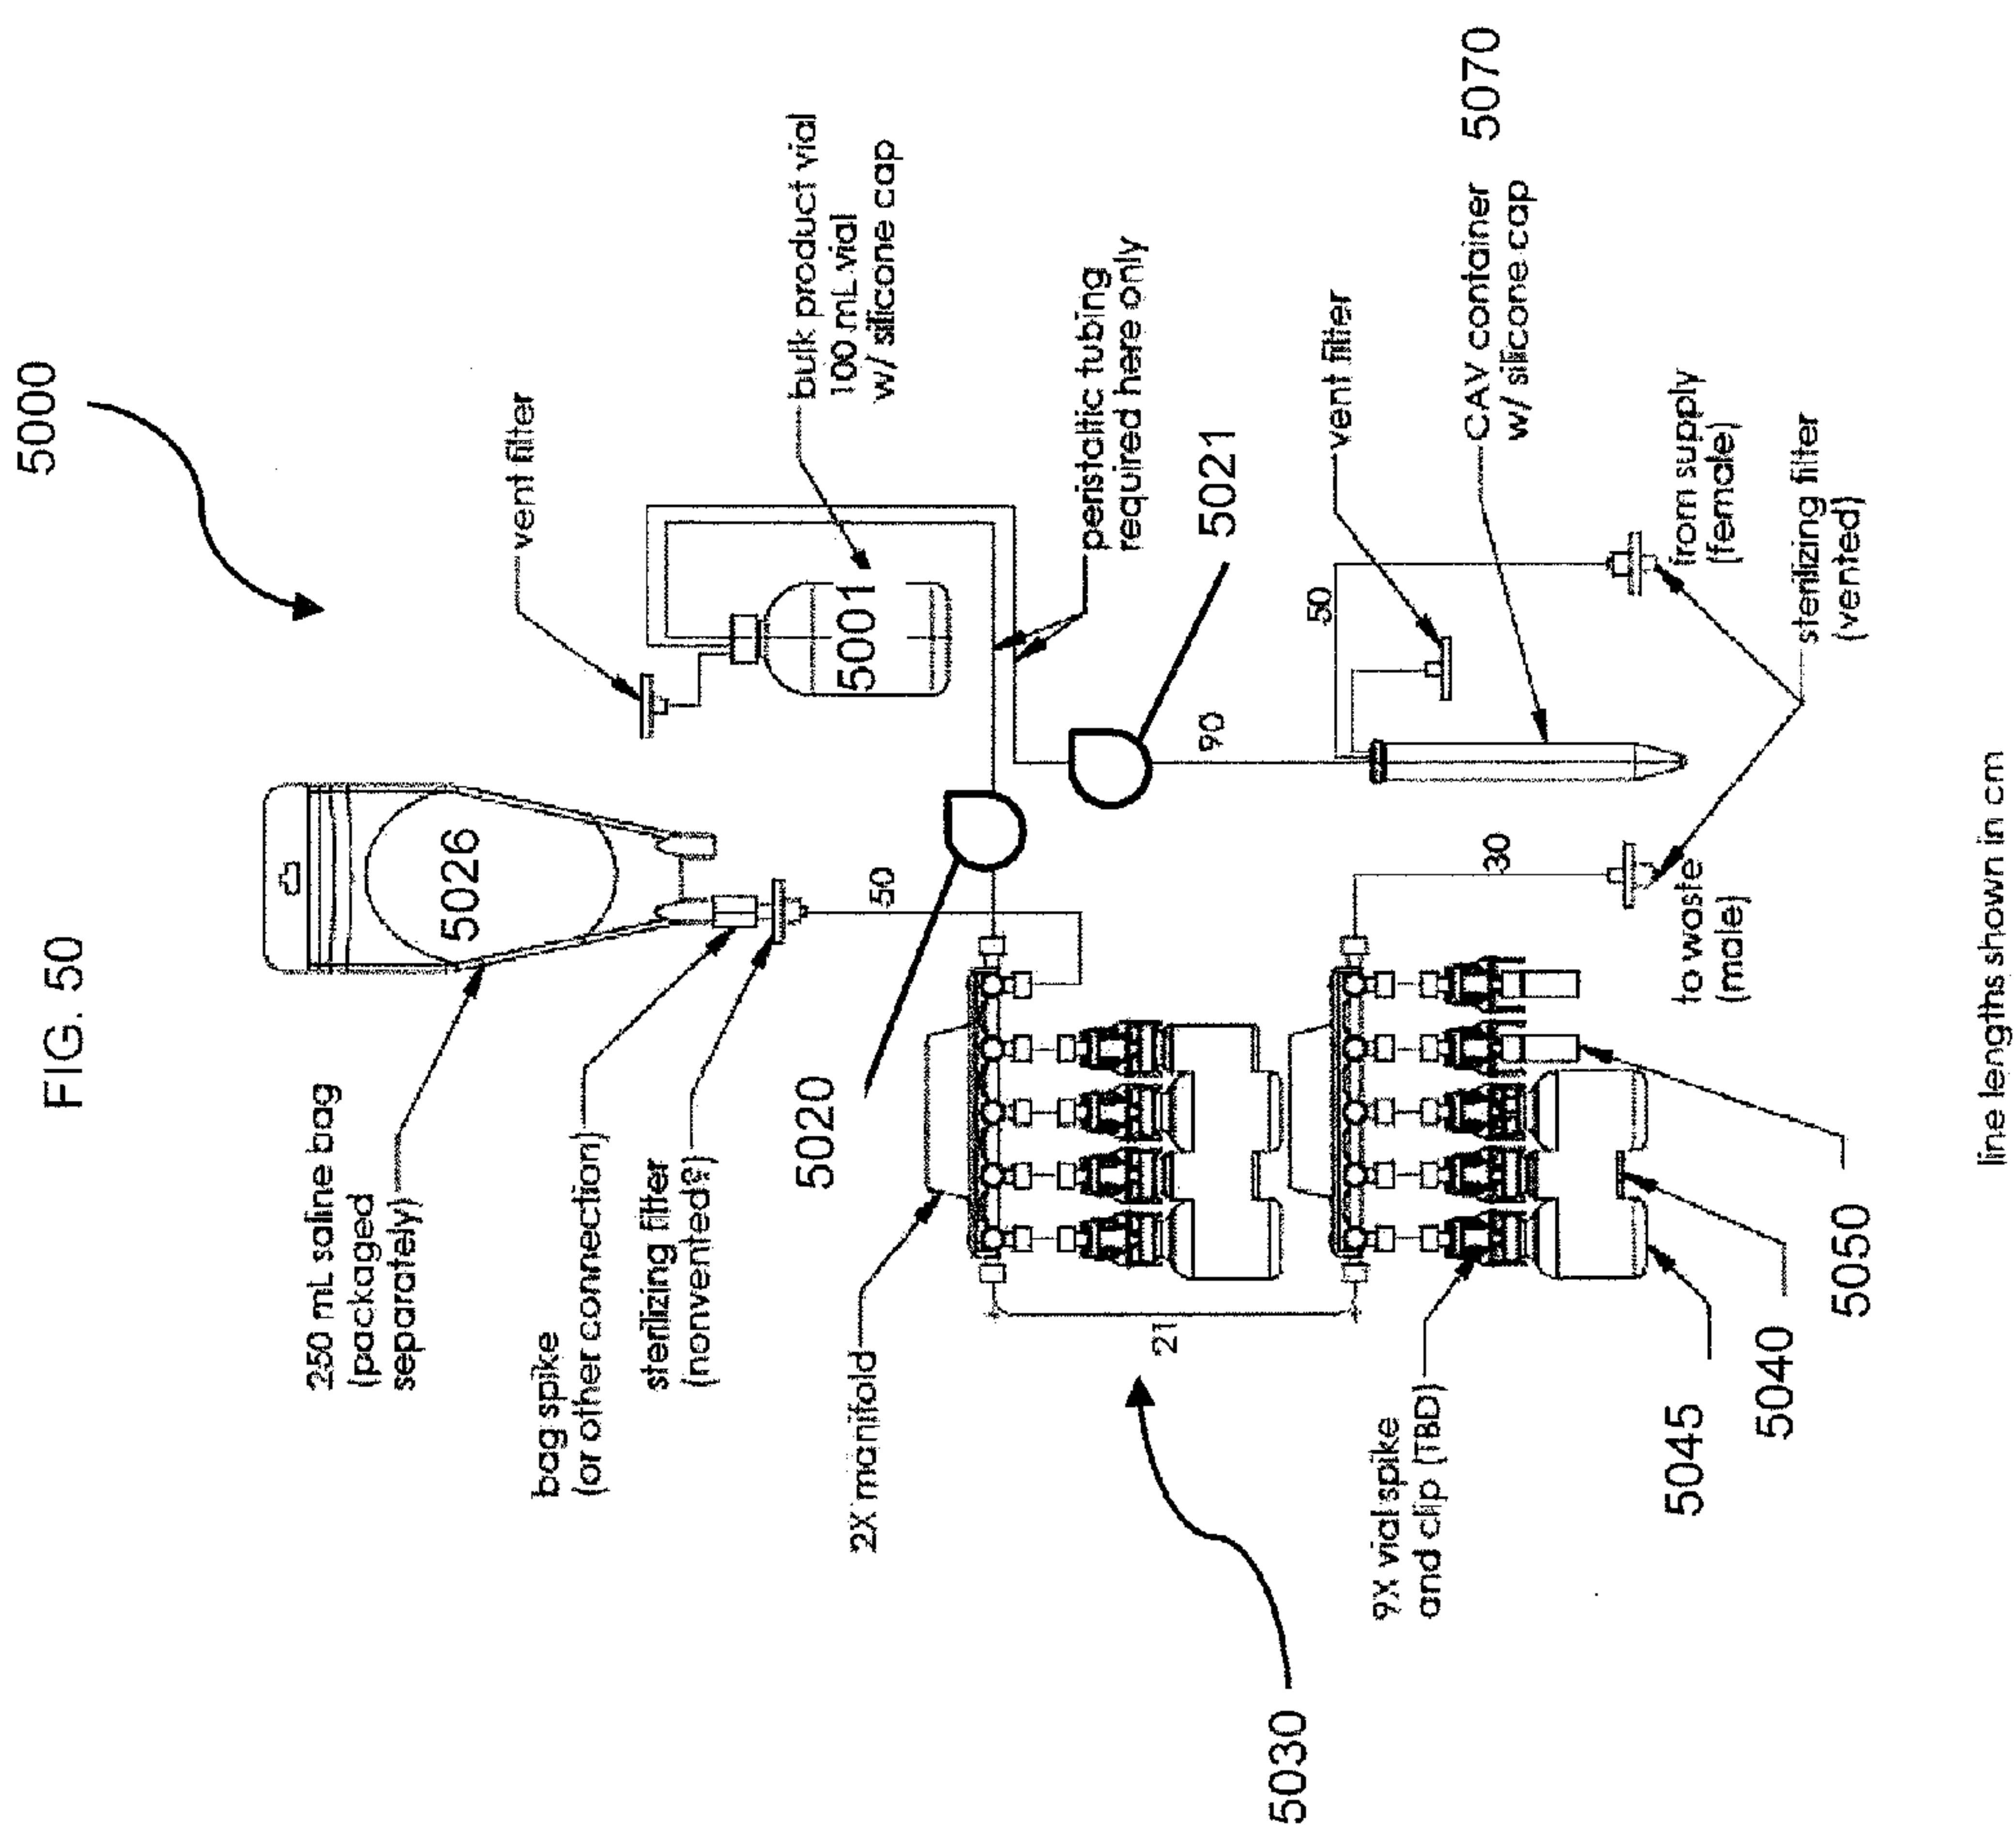



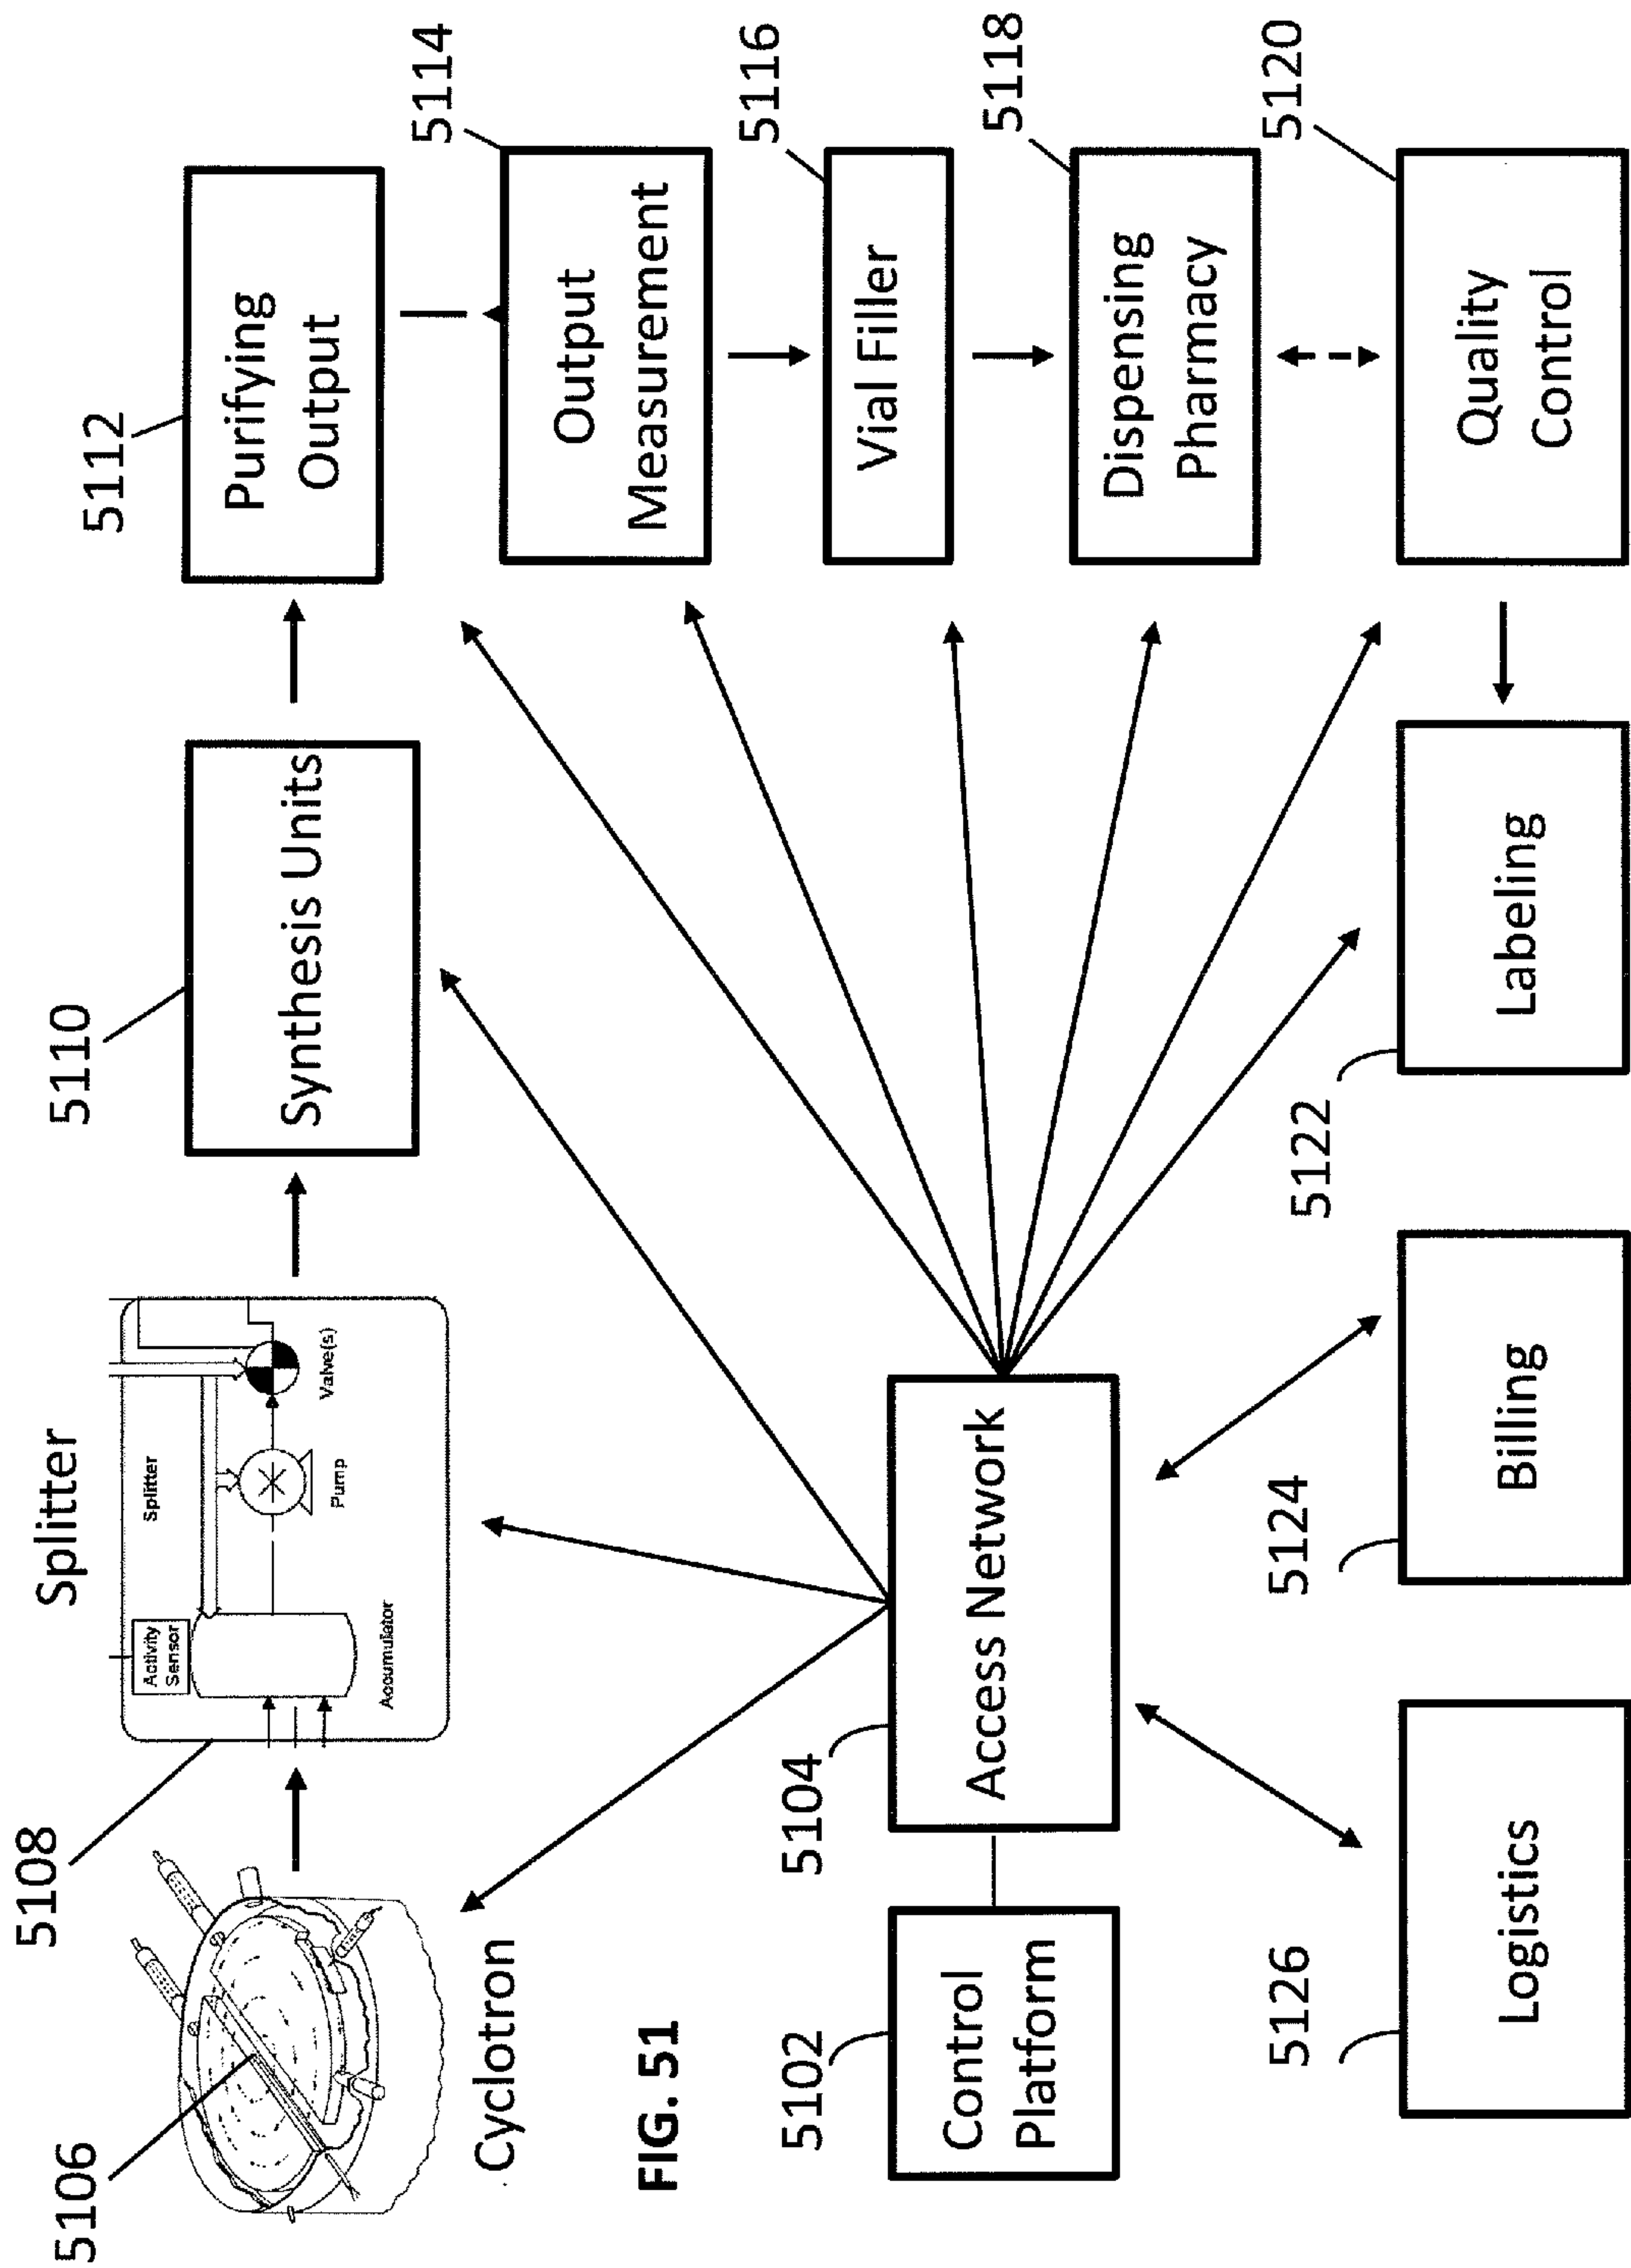


FIG. 52


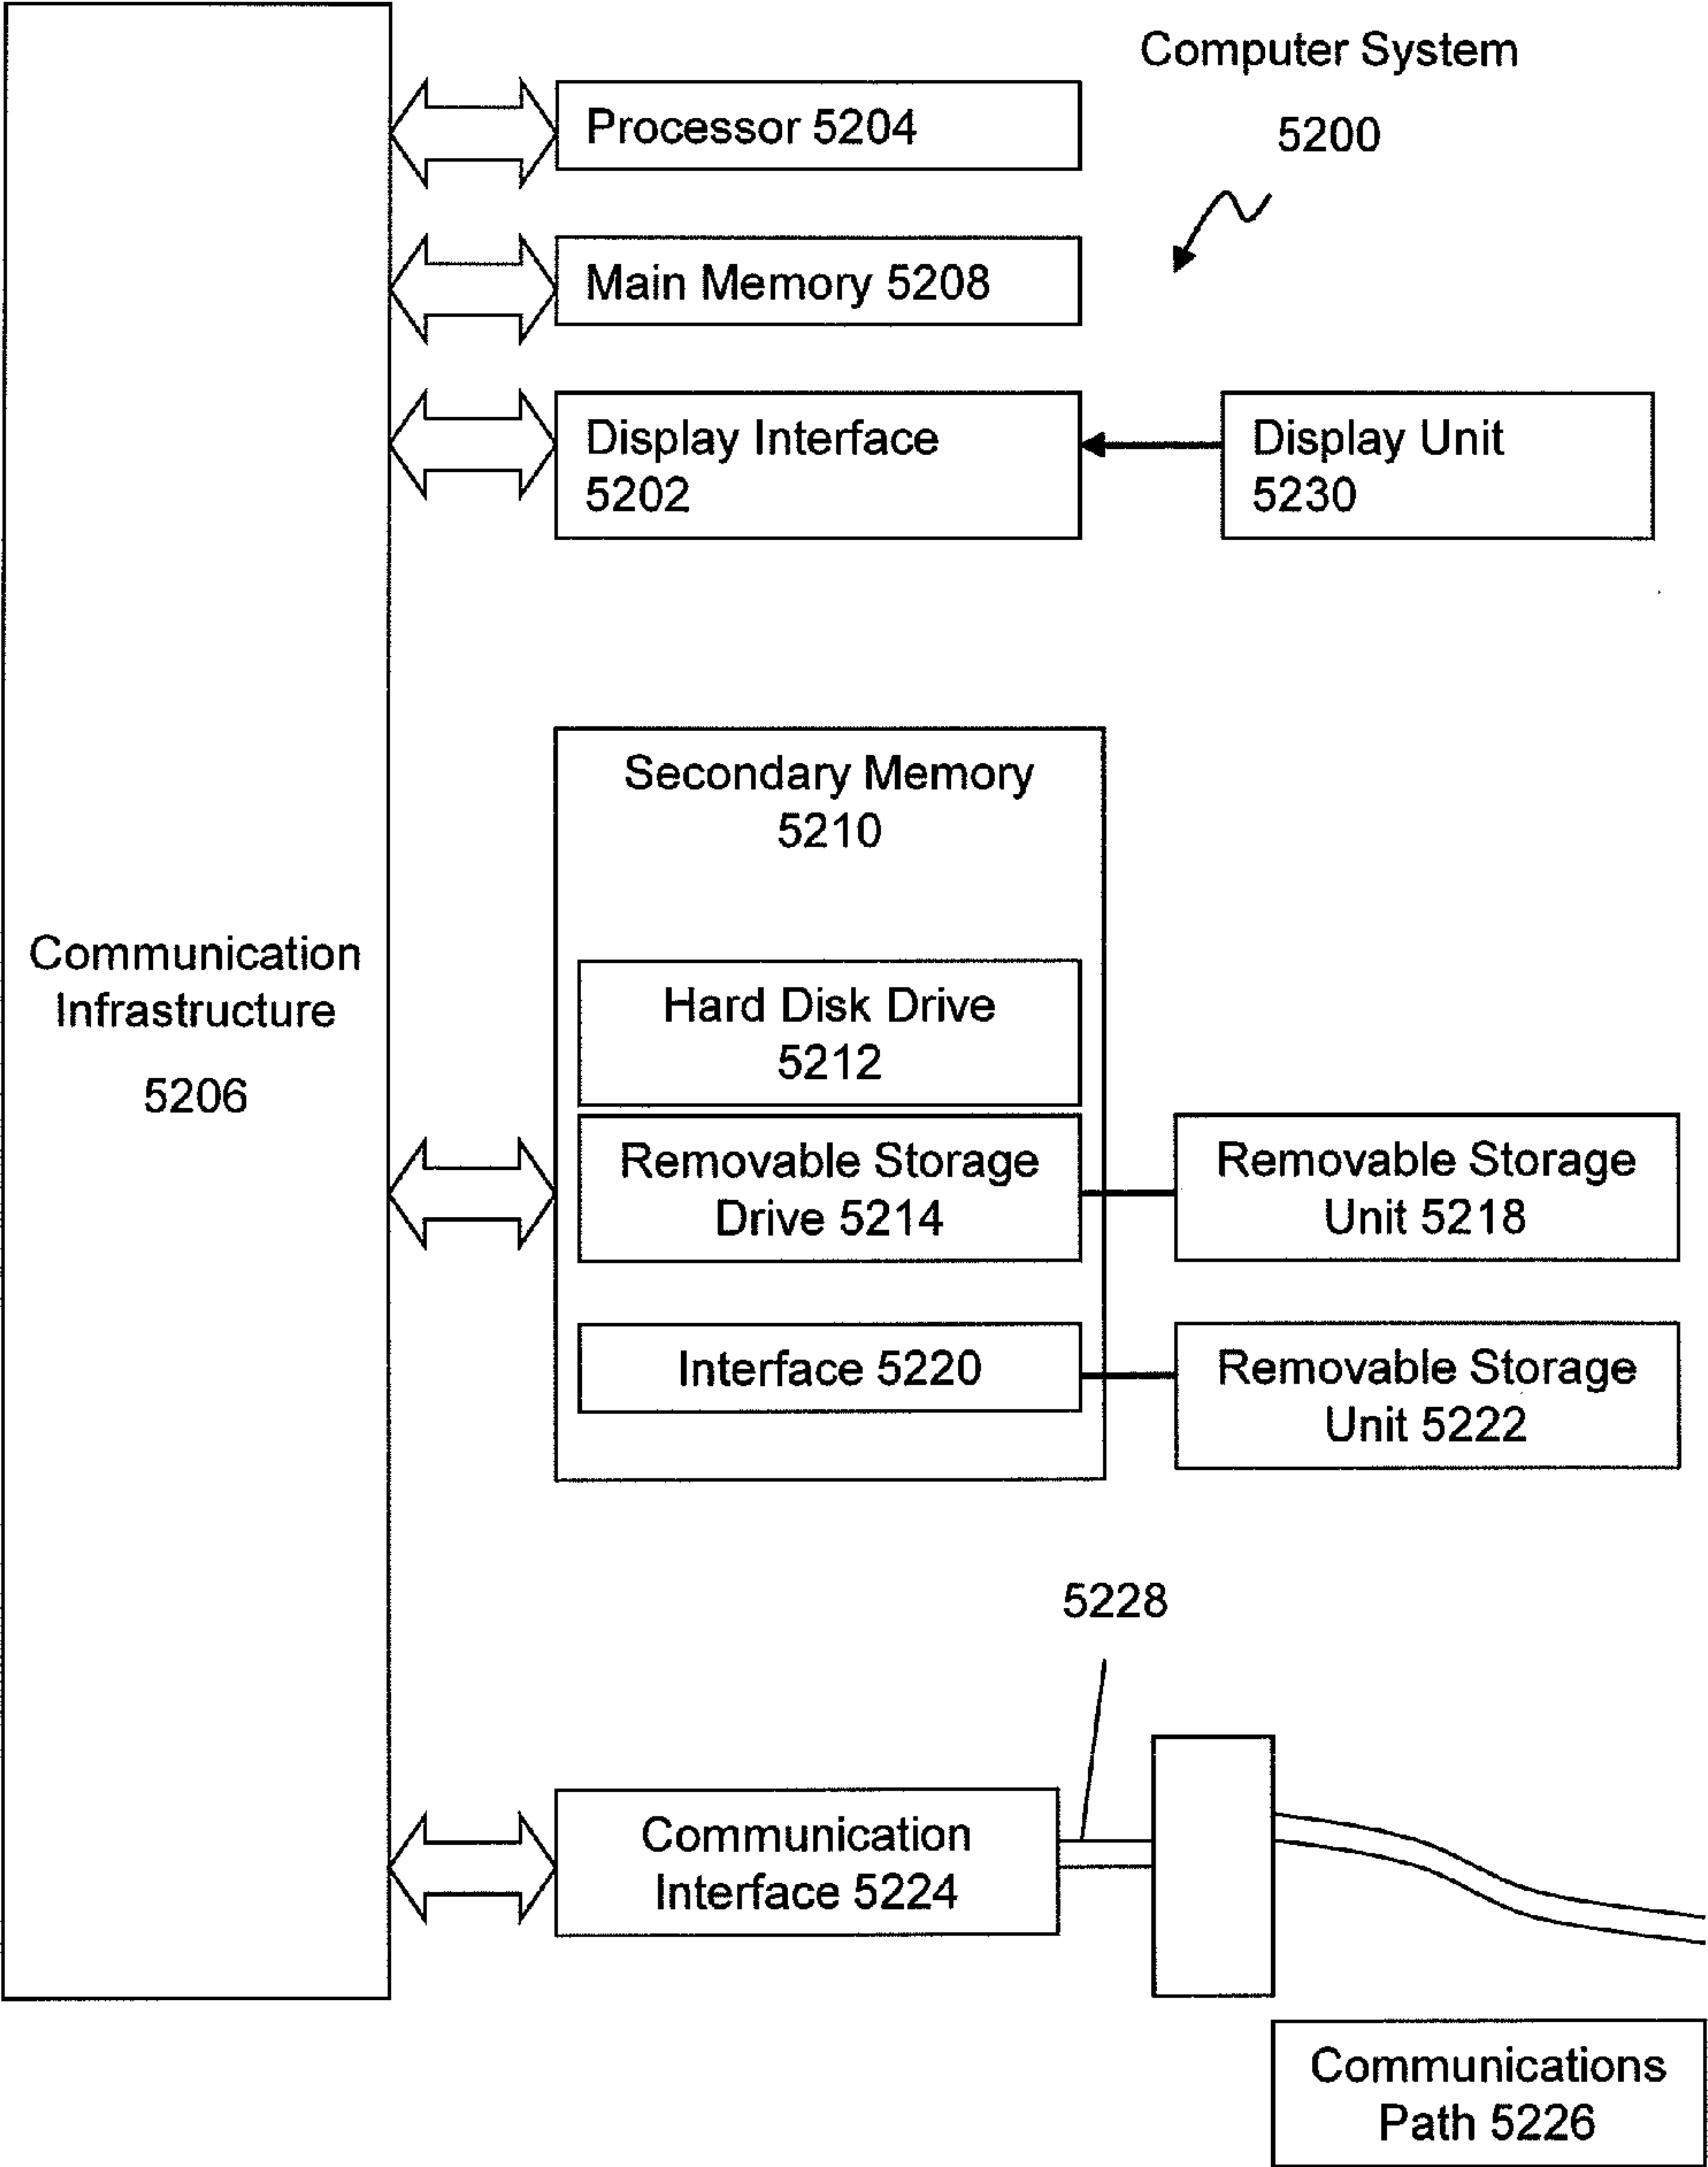




FIG. 53

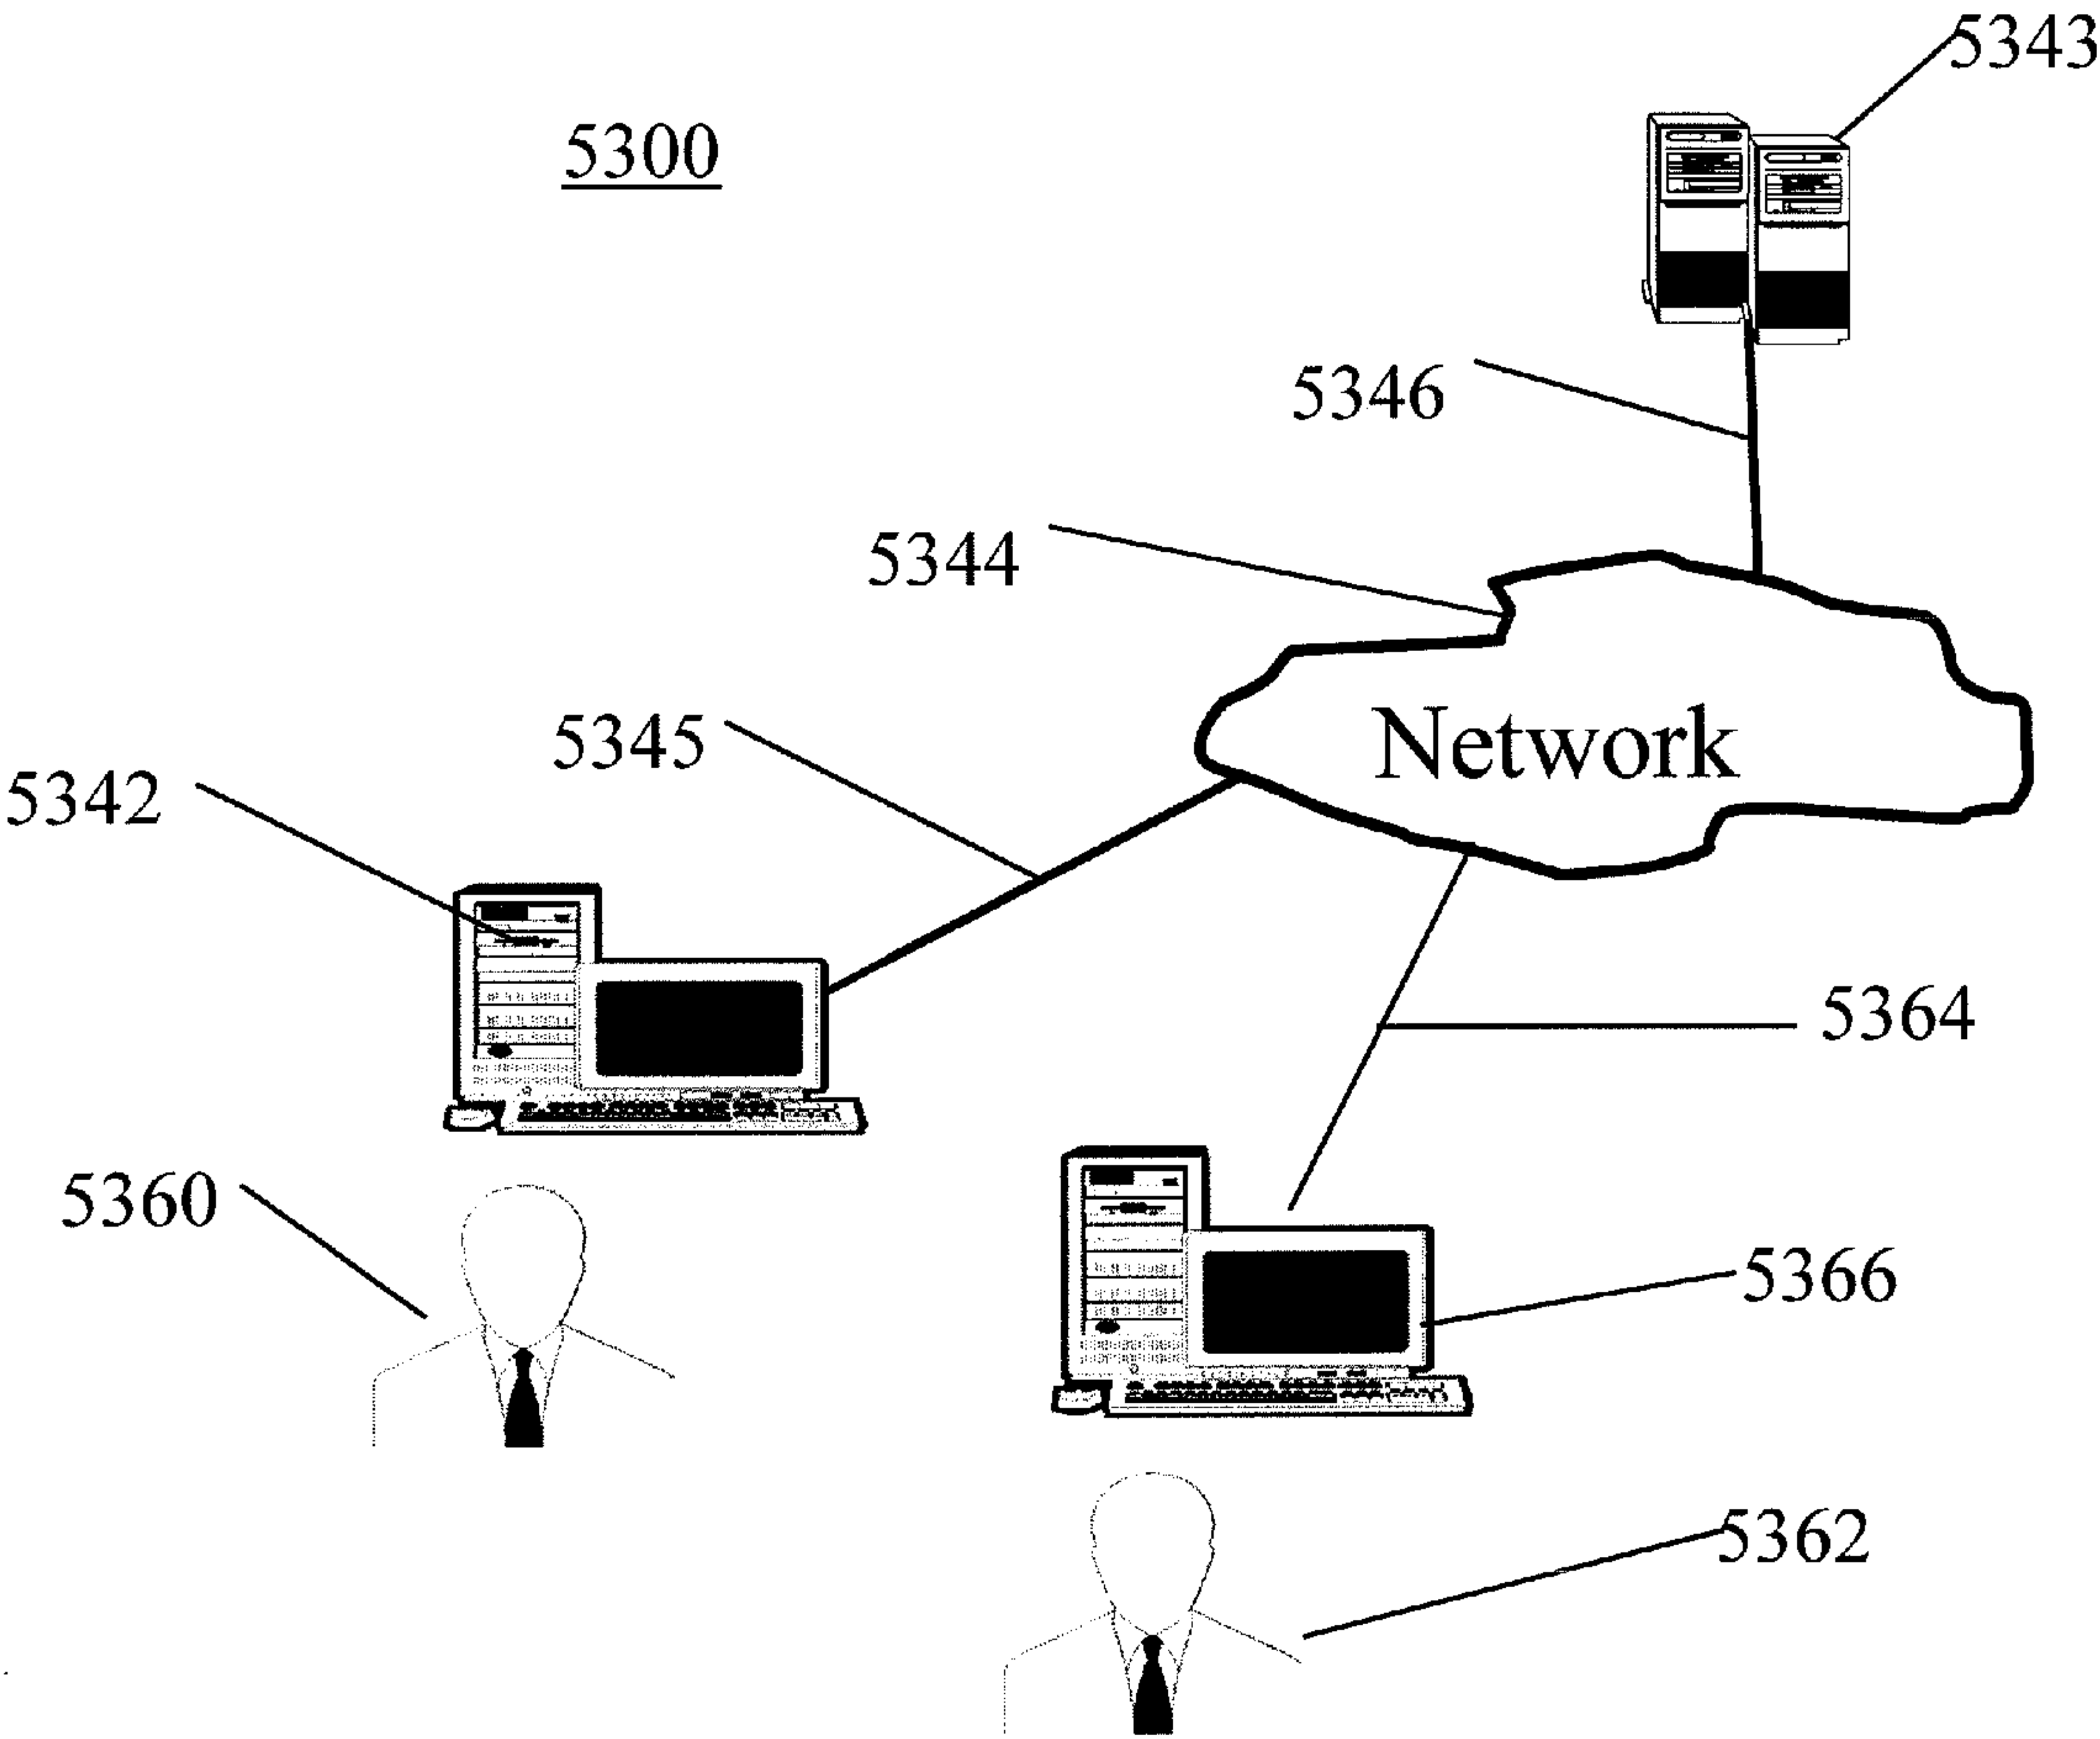

# SYSTEMS, METHODS AND DEVICES FOR PRODUCING, MANUFACTURING AND CONTROL OF RADIOPHARMACEUTICALS-FULL

CLAIM OF PRIORITY UNDER 35 U.S.C. §119

**[0001]** This application claims priority to U.S. Provisional Application No. 61/508,294 entitled “SYSTEMS, METHODS, AND DEVICES FOR PRODUCING, MANUFACTURING, AND CONTROL OF RADIOPHARMACEUTICALS” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,383 entitled “METHODS AND APPARATUS FOR FACILITATING THE PRODUCTION AND DISTRIBUTION OF RADIOPHARMACEUTICALS” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,374 entitled “SPLITTER SYSTEM AND METHODS OF USE THEREOF” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,382 entitled “MEMBRANE PUMPING SYSTEM AND METHOD IN A SURFACE CHANNEL FLUIDIC SYSTEM” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,402 entitled “RADIOPHARMACEUTICAL CZT SENSOR AND APPARATUS” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,394 entitled “ON-DEMAND PRODUCTION OF RADIONUCLIDES” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,359 entitled “CASSETTE REACTION VESSEL USING A CASCADE OF VALVELESS PRESSURE PUMPS” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,367 entitled “CASSETTE REACTION VESSEL” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,382 entitled “MODULAR CASSETTE SYNTHESIS UNIT” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,464 entitled “METHODS AND COMPOSITIONS FOR DRYING IN THE PREPARATION OF RADIOPHARMACEUTICALS” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,353 entitled “METHOD AND SYSTEM FOR AUTOMATED QUALITY CONTROL PLATFORM” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/553,029 entitled “METHOD AND SYSTEM FOR AUTOMATED QUALITY CONTROL PLATFORM—PART 2” filed on Oct. 28, 2011; U.S. Provisional Application No. 61/508,408 entitled “METHOD FOR SYNTHESIZING LABELED COMPOUNDS” filed on Jul. 15, 2011; U.S. Provisional Application No. 61/508,349 entitled “SYSTEM FOR RADIOPHARMACEUTICAL PREPARATION INCLUDING HIGH PERFORMANCE LIQUID CHROMATOGRAPHY MODULE” filed on Jul. 15, 2011; and U.S. Provisional Application No. 61/508,409 entitled “CLOSED VIAL FILL SYSTEM FOR ASEPTIC DISPENSING” filed on Jul. 15, 2011. Each of the preceding applications is incorporated by reference herein in its entirety.

## FIELD

**[0002]** Aspects presented herein relate to the field of fully or partially automated production of radiopharmaceuticals, and in particular to systems, methods, and devices for safe, secure, reusable, and flexible: 1) production of radionuclides; 2) accurate measurement and combination of produced radionuclides with other radiopharmaceutical raw materials to produce one or more output streams of radiopharmaceuticals; 3) delivery of the output streams for individual dose level distribution; and 4) provision of quality control contemporaneously with radiopharmaceutical dose production and distribution.

## BACKGROUND

**[0003]** Diagnostic techniques in nuclear medicine use radioactive tracers which emit gamma rays from within the body. These tracers are generally short-lived isotopes linked to chemical compounds which permit specific physiological processes to be studied. These compounds, incorporating radionuclides, are known as radiopharmaceuticals. They can be given by injection, inhalation or orally. In some diagnostic techniques, single photons are detected by a gamma ray sensitive camera, which can view organs from many different angles. The camera builds up an image from the points from which radiation is emitted; this image is enhanced by a computer and viewed by a physician on a monitor for indications of abnormal conditions.

**[0004]** Another recent development is Positron Emission Tomography (PET) which is a more precise and sophisticated technique using isotopes produced in a cyclotron, in which protons are introduced to the nucleus of a radioisotope, resulting in a deficiency of neutrons (i.e., becoming proton rich).

**[0005]** The nucleus of a radioisotope usually becomes stable by emitting an alpha and/or beta particle (or a positron). These particles may be accompanied by the emission of energy in the form of electromagnetic radiation known as gamma rays. This process is known as radioactive decay.

**[0006]** A positron-emitting radionuclide is introduced, usually by injection, and accumulates in the target tissue. As it decays, it emits a positron, which promptly combines with a nearby electron in the target tissue, resulting in the simultaneous emission of two identifiable gamma rays in opposite directions, each having an energy of 511 keV. These are conventionally detected by a PET camera and give a very precise indication of their origin. PET’s most important clinical role is in oncology, with fluorine-18 (F-18) as the tracer, since it has proven to be the most accurate non-invasive method of detecting and evaluating most cancers. Fluorine-18 (F-18) is one of several cyclotron producible positron emitters (including also, Carbon-11, Nitrogen-13, and Oxygen-15) used in PET for studying brain physiology and pathology, in particular for localizing epileptic focus, and in dementia, psychiatry and neuropharmacology studies. They also have a significant role in cardiology. F-18 in FDG (fluorodeoxyglucose) has become very important in detection of cancers and the monitoring of progress in their treatment, using PET. A radioactive product such as F-18 in FDG is a specific example of a radiopharmaceutical. Other radiopharmaceutical agents include, but are not limited to, F-18 Fluorothymidine (FLT), F-18 Fluoromisonidazole-3-fluoro-1-(2'-nitro-1'-imidazolyl)-2-propanol (MISO), F-18 Fluor Choline (FCH), and C-11 Acetate.

**[0007]** It is known in the related art to provide shielded containment systems for use in combining cyclotron produced radionuclides with non-radionuclide components to produce radiopharmaceuticals.

**[0008]** There are many drawbacks of these related art systems, including: 1) cyclotron production is often limited and does not allow the rapid production and distribution of short half-life radionuclides that are often needed; 2) typically only one radiopharmaceutical may be produced in a production run, after which various radionuclide raw material components and physical system components must be replaced and/or decontaminated, which can greatly delay the production process and/or make the process much less efficient; 3) many aspects of production of radiopharmaceuticals in such related art systems are not automated and/or may require time-con-



suming and/or awkwardly controlled hand production steps; 4) the radioactivity and/or quantities of the raw radionuclide and/or the produced radiopharmaceutical may be inaccurate and/or difficult to determine precisely; 5) necessary quality control to be performed on the output radiopharmaceutical products may be time-consuming, inaccurate, and/or require high levels of worker input/skill, further hampering production and/or timely delivery of the produced radiopharmaceuticals; 6) some or many aspects of the control, monitoring, and/or other production aspects may lack and/or hamper development of appropriate protections, such as shielding to minimize damage and maximize service life; 7) production/dispensing may be imprecise and/or inefficient for individual doses and/or may require inefficient or time consuming human intervention, as well as inefficient reuse of components and/or decontamination requirements; 8) control system software and hardware for overall operation and/or subsystem operation may be insufficient or not implementable; and/or 9) such existing systems may not provide or support use of remote and/or centralized data collection, control, and operation.

#### SUMMARY

**[0009]** Aspects presented herein overcome the above identified problems, as well as others, by providing systems, methods, and devices for producing radiopharmaceuticals that include: 1) generating radionuclides for use in production of radiopharmaceuticals, such as via use of a cyclotron (including enhanced systems, devices, and methods over the related art); 2) using the radionuclides generated to synthesize radiopharmaceuticals, and removing any unwanted products included with the generated radionuclides or radiopharmaceuticals or intermediate compounds in the synthesis (e.g., drying the generated radionuclides); 3) measuring the quantity and/or activity level of the synthesized radionuclides; 4) distributively delivering the radionuclides in appropriate quantities to a plurality of modular cassette synthesis units in a modular cassette subsystem for contemporaneous/parallel production of radiopharmaceutical output and to allow reuse and/or quick, safe, and disposable replacement of portions of the subsystem; 5) delivering appropriate quantities of non-radionuclide components to the plurality of modular cassette synthesis units as part of the contemporaneous/parallel production of radiopharmaceutical output; 6) upon production of the radiopharmaceutical output from the plurality of modular cassette synthesis units, measuring the quantity and activity level of each stream of radiopharmaceutical output (e.g., one or more radioactivity sensors or dose calibrators); 7) purifying the radiopharmaceutical output (e.g., removing any unwanted products included with the generated radionuclides, such as by drying and/or deprotecting the generated radionuclides and/or radiopharmaceuticals or intermediate compounds, which may optionally include use of one or more disposable columns); 8) distributively dispensing bulk product in one or more sterile vials or manufactured dose containers; 9) optionally automatically producing labeling and/or dose related information for use with the doses; 10) performing automated quality control on one or more extracted samples from the produced radiopharmaceutical output; and 11) providing software and/or hardware controls for overall and various sub-portion operation that include suitable radiation and other damage and contaminant resistant features and that allow for optional remote data collection and troubleshooting, communication, and/or control.

**[0010]** In one example implementation, a related art housing and other features typically used to produce a single radiopharmaceutical production run that may include significant human intensive input is used to house a plurality of modular subsystem components that automate and improve speed and accuracy of production, allow multiple radionuclide products to be produced contemporaneously/in parallel, and enable efficient and quick substitution of product runs.

**[0011]** In one example implementation, for reagent and synthesis operation, internal related art shielded openings used for components for a single product run are replaced with multiple subsystems that two or more contemporaneous/parallel production operations. In addition, cooperation among other system components allows increased production by allowing increased efficiency of feed and accuracy of both characteristics and volume of radionuclide and other raw material input to the production process.

**[0012]** Aspects presented herein include enhanced and/or alternative systems, devices, and methods for production and improved quality and quantity of raw radionuclides usable in the manufacture of radiopharmaceuticals.

**[0013]** Increase in automation of portions of operation, as well as improvement, reduction of size and cost, and advancement of operation of cooperating portions of reagent and synthesis operations results in the both increased speed and accuracy of production and decreased human exposure during the process. Subsystem components may be modularized, such by use of cassettes, and designed to allow interactive use that enables quick and simplified replacement/disposal of modules to, among other things, reduce contamination, enable quick and simplified input of selected raw material feeds, and enable simplified substitution of entire radiopharmaceutical processes.

**[0014]** Aspects include devices, systems, and methods for both measuring activity level of radionuclides and accurately determining the volume of such materials throughout the system increase both efficiency and quality of output. Such devices and systems also have enhanced robustness of operation in radiation and contaminant exposed environments.

**[0015]** In one example implementation, 10 of 11 steps in a quality control process are automated to run in parallel/contemporaneously and to run contemporaneously with dispensing and/or other operations of the manufacturing process, so as to reduce the time from manufacture to delivery of each radiopharmaceutical. This automated approach reduces delay, decreases the need for human resources (and thereby costs associated with human resource skills, as well as resulting in reduction in human errors), and enables more standardized quality control output.

**[0016]** In one example implementation, post radiopharmaceutical production manufacturing and/or purification processes are used to produce higher quality products more quickly than the related art. Such features may include, for example, use of high performance liquid chromatography (HPLC), low pressure chromatography, flash chromatography as well as types of Sep-Pak purification and isolation processes, and disposable columns.

**[0017]** In one example implementation, dose dispensing is automated and highly accurately controlled through use of subsystem components, and may be modularized, such as via use of cassettes, to allow interactive use that enables quick and simplified replacement/disposal of modules to, among other things, enable quick and simplified substitution of portions of or entire dose dispensing processes. In some varia-



tions, the accuracy of feeds is enhanced by use of robust detection devices, systems, and methods in conjunction with automated generation of information that enable accurate dose dispensing, for example, contemporaneously with accurate labeling and other information generation for dose dispensation over the lifetime of the radiopharmaceutical.

**[0018]** In example implementations, operations of the overall system, as well as subsystem features, may be controlled by one or more software and hardware control systems and methods of operation. Various operations, inputs, and/or output may thereby easily be centrally/remotely collected and/or controlled.

**[0019]** Additional advantages and novel features relating to aspects presented herein will be set forth in part in the description that follows, and in part will become more apparent to those skilled in the art upon examination of the following or upon learning by practice thereof.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0020]** Aspects presented herein will become fully understood from the detailed description given herein below and the accompanying drawings, which are given by way of illustration and example only and thus not limited with respect to aspects of the present invention, wherein:

**[0021]** FIG. 1 presents a representative diagram of various portions of an example system in accordance with aspects of the present invention;

**[0022]** FIG. 2 shows a basic system schematic of one example of an overall system architecture, in accordance with aspects of the present invention;

**[0023]** FIG. 3 shows a view of example synthesis units in an example housing and including an example splitter in accordance with aspects of the present invention;

**[0024]** FIGS. 4A and 4B contain partial cutaway views of example shielded hot cells housing vial filler units for use in determination of final product activity (e.g., radiation) levels and dispensing production vials, in accordance with aspects of the present invention;

**[0025]** FIG. 5 shows an example dispensing unit, in accordance with aspects of the present invention;

**[0026]** FIGS. 6A and 6B present cutaway views of an example quality control unit or subsystem for performing automated quality control on one or more samples extracted from the produced radiopharmaceutical output, in accordance with aspects of the present invention;

**[0027]** FIG. 7 illustrates a system diagram in accordance with aspects presented herein;

**[0028]** FIG. 8 shows an example FDG schematic using isolation valves around a reaction vessel and pressure pumping for fluid transfer, in accordance with aspects of the present invention;

**[0029]** FIG. 9 shows an example FDG process chart, in accordance with aspects of the present invention;

**[0030]** FIG. 10 shows the Example F-18 Product 1A process schematic using isolation valves around a reaction vessel and pressure pumping for fluid transfer, in accordance with aspects of the present invention;

**[0031]** FIG. 11 shows an example process chart for Example F-18 Product 1A, in accordance with aspects of the present invention;

**[0032]** FIG. 12 shows an example device for enhanced generation of F-18 radionuclide on demand, in accordance with aspects of the present invention;

**[0033]** FIGS. 13-21 illustrate examples of activity and/or volume sensors in accordance with aspects presented herein;

**[0034]** FIGS. 22-28 show examples of a splitter subsystem in accordance with aspects of the present invention;

**[0035]** FIG. 29 illustrates an example user interface in accordance with aspects presented herein;

**[0036]** FIG. 30 contains a Photostat of example pump detail in accordance with aspects of the present invention;

**[0037]** FIGS. 31 and 32 illustrate an example membrane pump in accordance with aspects presented herein;

**[0038]** FIG. 33 illustrates an example cascade pump in accordance with aspects presented herein;

**[0039]** FIGS. 34-36 illustrate views of one example Multi-Synth devices, in accordance with aspects of the present invention;

**[0040]** FIG. 37 shows a view of an example of a synthesis cassette and reagent pack installed on an example module, in accordance with aspects of the present invention;

**[0041]** FIG. 38 shows an example of a synthesis cassette, in accordance to aspects of the present invention;

**[0042]** FIGS. 39-40 present an overview of one example synthesis module design approach, in accordance with aspects of the present invention;

**[0043]** FIG. 41 shows an exploded view of various portions of an example synthesis cassette, in accordance with aspects of the present invention;

**[0044]** FIGS. 42 and 43 illustrate exploded views of various features of an example reagent pack, in accordance with aspects of the present invention;

**[0045]** FIG. 44 shows an example of bent foil flaps produced using angled piercing posts, in accordance with aspects of the present invention;

**[0046]** FIG. 45 shows a schematic of an example HPLC system module in accordance with aspects of the present invention;

**[0047]** FIGS. 46 and 47 present an overview of one example design approach to the HPLC/Low Pressure chromatography/Flash chromatography as well as types of Sep-Pak purification module in accordance with aspects of the present invention;

**[0048]** FIGS. 48, 49, and 50 show aspects an examples of vial fillers, in accordance with aspects presented herein;

**[0049]** FIG. 51 presents a representative diagram of various portions of an example system in accordance with aspects presented herein; and

**[0050]** FIGS. 52 and 53 show a representative diagram of an example computer system for use in accordance with aspects of the present invention.

#### DETAILED DESCRIPTION

**[0051]** Aspects presented herein overcome the above identified problems, as well as others, by providing systems, methods, and devices for producing radiopharmaceuticals that include: 1) generating radionuclides for use in production of radiopharmaceuticals, such as via use of a cyclotron (including enhanced systems, devices, and methods over the related art); 2) using the radionuclides generated to synthesize radiopharmaceuticals, and removing any unwanted products included with the generated radionuclides or radiopharmaceuticals or intermediate compounds in the synthesis (e.g., drying the generated radionuclides); 3) measuring the quantity and/or activity level of the synthesized radionuclides; 4) distributively delivering the radionuclides in appropriate quantities to a plurality of modular cassette synthesis units in



a modular cassette subsystem for contemporaneous/parallel production of radiopharmaceutical output and to allow reuse and/or quick, safe, and disposable replacement of portions of the subsystem; 5) delivering appropriate quantities of non-radionuclide components to the plurality of modular cassette synthesis units as part of the contemporaneous/parallel production of radiopharmaceutical output; 6) upon production of the radiopharmaceutical output from the plurality of modular cassette synthesis units, measuring the quantity and activity level of each stream of radiopharmaceutical output (e.g., via one or more hot cells); 7) purifying the radiopharmaceutical output (e.g., removing any unwanted products included with the generated radionuclides, such as by drying and/or deprotecting the generated radionuclides and/or radiopharmaceuticals or intermediate compounds, which may optionally include use of one or more disposable columns); 8) distributively dispensing individual doses in one or more sterile vials; 9) optionally automatically producing labeling and/or dose related information for use with the doses; 10) performing automated quality control on one or more extracted samples from the produced radiopharmaceutical output; and 11) providing software and/or hardware controls for overall and various sub-portion operation that include suitable radiation and other damage and contaminant resistant features and that allow for optional remote data collection, communication, and/or control.

**[0052]** In a radiopharmaceutical production facility, a cyclotron or linear accelerator may be used to prepare a material containing a radioisotope of interest which is delivered to a synthesis system. The radioisotope may emit one or more kinds of radiation, including electrons, positrons, gamma rays/x-rays, protons, neutrons, alpha particles, and other possible nuclear ejecta. In one example, a radioisotope, when added to other materials to be administered to a subject, may emit a positron, which then annihilates with an electron, for example, in human tissue, to produce gamma rays.

**[0053]** FIG. 1 presents a representative diagram of various portions of an example system in accordance with aspects presented herein. As shown in FIG. 1, the example system **100** includes a cyclotron or other device **105** for generating radionuclides (e.g., F-18) for use in production of radiopharmaceuticals; a splitter **110** for measuring (e.g., quantity and radioactivity) and accurately dividing the generated radionuclides into split streams for further production; one or more synthesis units **115** for further processing the radionuclides and/or other products to be combined with the radionuclides (e.g., modular cassette unit(s) to produce a radiopharmaceutical containing the radionuclides); an output measurement component **120** for measuring (e.g., quantity and radioactivity) the output from the synthesis unit(s); a purifying component for purifying the output (e.g., removing any unwanted products included with the generated radionuclides, such as by drying and/or deprotecting the generated radionuclides and/or radiopharmaceutical or intermediate compound, which may optionally include use of one or more disposable columns); one or more dispensing units **130**, such as for distributively dispensing individual doses into one or more sterile vials; a quality control unit **135** for performing automated quality control on one or more extracted samples from the produced radiopharmaceutical output; an optional labeling component **140** for automatically producing labeling and dose related information for use with the doses output; an optional connection to a dispensing pharmacy that may be located remotely; and software and hardware control features

**150**, including network **155** (e.g., the Internet) and remote hardware and/or software components **160** for overall and various sub-portion operational control that optionally may allow for remote data collection, communication, and/or control.

**[0054]** For example, the amount of radiopharmaceutical product needed in a predetermined amount of time may be determined, the determined amount of radiopharmaceutical product may be produced using any combination of cyclotron **105**, splitter **110**, synthesis unit **115**, purifying output **125**, output measurement **120**, vial filler, quality control, and labeling. The predetermined period of time may be a day. Thus, orders for the following day may be determined so that the correct amount of radiopharmaceutical product can be determined, produced, and distributed for use within the following day. The amount of radiopharmaceutical product produced for a corresponding remote dispensing pharmacy **145** may be transmitted to the dispensing pharmacy **145** in bulk quantity, and the corresponding amounts may be indicated to a pharmacist in order to draw the correct individual doses. Using software control **150**, the dose may be automatically drawn and corresponding information provided to the pharmacist. Software control may receive information for a plurality of doses that will be required in the predetermined period of time and automatically begin the radiopharmaceutical production process without further user input. However, a user interface may be provided to receive user input regarding the desired amounts at the location of the splitter **110** and synthesis units **115**. Software control **150** may receive information for required doses from a plurality of remote locations and combine the received information in order to produce the total amount of required radiopharmaceutical product. Thereafter, information for each of the required doses may be forwarded to the corresponding dispensing pharmacy **145** from which the dose should be drawn. As radio decay information is critical for the dispensing pharmacist to draw the correct individual dose, the automated system may take into account the production information for the radiopharmaceutical product was finished when indicating the amount for the individual dose. The automated system may further take into account the day or time at which each of a plurality of individual dose are intended to be used when determining the amount to be produced.

**[0055]** Hardware and/or software components **150** and **160** may comprise, for example, one or more personal computers (PCs), minicomputers, mainframe computers, microcomputers, telephonic devices, or wireless devices, such as a personal digital assistants ("PDA") or other hand-held wireless devices for receiving, storing, and processing data. The hardware and/or software may include a processor and a repository for data and/or couplings to a repository for data, via, for example, a network, such as the Internet or an intranet. The couplings may include, for example, wired, wireless, or fiberoptic links.

**[0056]** In one example implementation in accordance with aspects presented herein, the overall system architecture may include three major subsystems: a drug synthesis subsystem that may include a plurality of modules and cassettes, a fluid supply, a gas supply, a vacuum supply, and fluid recovery components; a splitter that may be housed outside/behind the mini-cell; and power and control electronics unit that may be housed outside/behind the mini-cell.

**[0057]** FIG. 2 shows a basic system schematic **200** in accordance with one such example implementation. FIG. 2 illus-



trates a supply line **201** that receives radionuclides from a radionuclide generator, e.g., a cyclotron, and supplies the radionuclides to a splitter **202**. Supply line **201** may be replaceable. Splitter **202** is illustrated adjacent to mini cell **203**, and may be located in any shielded area outside of the mini cell **203**. Splitter receives radionuclides from one or more cyclotrons and divides and routes the solution to a plurality of modules **204** and modular cassettes **205** comprised in the synthesis unit. Splitter may comprise an accumulator **206** for accumulating the received radionuclides, and a sensor such as an activity sensor **207**, that measure the liquid volume and activity level of the received radionuclides. Activity sensor may comprise a CAV sensor as described in further detail in connection with FIGS. 12-18.

[0058] Once received, the radionuclide may remain in the accumulator until a product demand is identified. At that point, the volume of liquid required may be calculated and routed, e.g., pumped, to one of the plurality of cassettes in the synthesis unit or mini cell **203**. Splitter may comprise a pump **208** and valve **209** for routing the required amount of radionuclides to the appropriate cassette. An example splitter is described in additional detail in FIGS. 22-28.

[0059] Mini cell **204**, also referred to interchangeably herein as a synthesis unit, may comprise a plurality of modules **204** and cassettes **205** that are used to formulate the product. For example, six modules **204** and six cassettes **205** may be installed in a mini-cell **204**. Mini-cell **204** may comprise a bulk fluid supply **218a, b, c, and d**, a gas supply **219**, and a vacuum supply **220**. Mini cell **204** may also comprise a vent line **222** connecting each of the cassettes **205** to the exterior of the mini cell **204**. A synthesis unit supply line **221** may connect each of these sources to each of a plurality of synthesis modules **204**. The components comprised within the synthesis cassette may be configured in a lab-on-a-chip architecture, comprising all necessary reagents and supporting all synthesis reaction processes. The cassettes may receive radionuclides as a primary input and provide the pharmaceutical product as the primary output. Each cassette **205** is supported by a corresponding module **204** that provides the necessary connections for required bulk gases or fluids, along with proximity or physical interfaces for heating, cooling, and sensing. The provision of common solvents that tend to be used in large quantities via bulk containers reduces the required volume for each of the cassettes. This minimizes the size of each of the cassettes and maximizes the number of cassettes that can be provided in each mini cell.

[0060] Mini cell **203** may further comprise a sensor, e.g., an activity sensor **223**.

[0061] At least one of the plurality of cassettes **205** and/or the plurality of modules **204** may comprise HPLC components for performing product purification. The HPLC component, therefore, may also comprise a connection to at least one of the other cassettes for receiving an output product from the cassette for purification.

[0062] Exit lines **214** and **215** may connect directly to each of the cassettes **205**. One exit line **215** may receive liquid waste from each of the cassettes, and another exit line **214** may recover  $\text{H}_2^{18}\text{O}$ .

[0063] A product supply line **216** may connect each of the cassettes internal to the mini cell to the exterior of the mini cell, e.g., to a vial filler **217** exterior to the mini cell **204**.

[0064] The system **200** may further include power and control electronics **210**. The power and control electronics is illustrated in a location outside mini-cell **203** and splitter **202**.

The power and electronics **210** provide power to system components, receive sensor signals from system components, provides command/control signals to system components, executes system command and control, and provides a system user interface. This component **210** may interface the system **200** with a main power supply **211**, a remote monitor **212**, and component **213** for receiving user input and outputting information to users.

[0065] The supply lines throughout the system may be replaceable in order to prevent contamination and to enable quick turnaround between different products. For example, supply lines **201**, exit lines **214** and **215**, product supply lines **216**, and synthesis unit supply line **221** may comprise a replaceable line.

[0066] Fluid recovery may comprise separate compartment for waste and for—water.

[0067] The system may comprise an off state when no power is supplied to the system components, a standby state when power is supplied to the system components and system functions are not available to the splitter **202** and product synthesis subsystems, an operational state when system functions are available to the splitter **202** and product synthesis subsystems, and a service state during which system subsystems are not available to the splitter **202** and product synthesis subsystems and during which system components are selectively enabled and disabled in order to perform tests, repair components, or perform maintenance actions. The power and control electronics **210** may exist at the operational system level, as one of its functional roles may be to command and control the operation of the splitter **202** and the modules **204** within the synthesis product subsystems.

[0068] At the product synthesis subsystem level, the components comprised in the mini cell **203** may likewise comprise at least a standby state, an operational state, and a service state. At the Module **204** level, the components may comprise at least a standby state a ready state where module functions are available for performing product synthesis, and operational state, and a service state. At the splitter **202** level, the components may likewise comprise a standby state, a ready state, an operational state, and a service state.

[0069] Among others, such radiopharmaceutical products may include Fluorodioxylucose (FDG), F-18 Product 1A, Fluorothymidine (FLT), Fluoromisonidazole (F-Miso), F-18 Product 2, F-18 Product 1B, and F-18 Product 3.

[0070] Synthesis for certain products may be accomplished without the use of HPLC columns, such as the synthesis of FDG.

[0071] FIGS. 3-6 show views of example implementations of various aspects in accordance with the example system of FIG. 1. FIG. 3 shows an example splitter **310** located atop a housing **300** that contains a plurality of synthesis units **315**. The housing **300** may, for example, have been originally designed for handling a single synthesis portion, and, in accordance with aspects presented herein, multiple synthesis units **315**, which may, for example, include cassette and other interchangeable subportions, may be sized and designed to fit the space originally designed for a single synthesis unit. Among other things, this approach to using multiple synthesis units within a single housing may allow multiple parallel processing of one or more radiopharmaceuticals, the same or different, for example, to be produced contemporaneously.

[0072] FIGS. 4A and 4B contain partial cutaway views of example vial fillers for use in determination of final product activity (e.g., radiation) levels, in accordance with aspects



presented herein. The example hot cells may contain, for example, one or more component or subsystems for measuring product activity, such as by using containers for which activity level may be monitored using monitoring devices to determine activity level and volume (via relative activity level at differing locations). Such monitoring devices may include, for example, one or more specially designed CdZnTe (“CZT”) solid state detectors for columnally measuring radiation contained within a container. The example hot cells may also contain dispensing units.

[0073] FIG. 5 shows another example dispensing unit **500**, in accordance with aspects presented herein, such as a vial filling device or subsystem. The vial filling device is illustrated having a plurality of vials **502** that may be in different sizes. The vial filler **500** may include a weighing module **504**, a pump **506** for filling a vial with a predetermined amount of radiopharmaceutical product, a dilution bag for diluting the radiopharmaceutical product, and a sensor **510**. The sensor may comprise a CAV sensor module and a CAV sensor disposable portion. FIGS. **21a-c**, for example, illustrate an example sensor and weighing component. The pump **506** may comprise a dual pumphead peristaltic pump.

[0074] FIGS. **6A** and **6B** present cutaway views of an example quality control unit or subsystem **600** for performing automated quality control on one or more samples extracted from the produced radiopharmaceutical output, in accordance with aspects presented herein. Among others, such quality control may comprise tests to confirm radiochem identity, radiochem purity, pH, product clarity, radionuclidic identity, kryptofix, and a BET test. Additional aspects of a quality control platform are disclosed in additional detail in U.S. Provisional Application No. 61/508,353 titled “Method and System for Automated Quality Control Platform,” filed on Jul. 15, 2011, the entire contents of which are hereby incorporate by reference herein.

[0075] FIG. 7 illustrates a system overview diagram **700**. FIG. 7 illustrates multiple lines **702** extending from a radionuclide generator **704**, such as a cyclotron. The different lines **702** correspond to different radionuclides. For example, **11C** is illustrated as connecting directly to a synthesis box selector **706a** that distributes the active product comprising **11C** to a minicell **708**.

[0076] A control unit **710** controls each of the radionuclide generator, the splitter, the synthesis unit selectors **706a**, **706b**, and the minicell **708**. Selectors **706a** and **706b** may be provided between the radionuclide generator **704** and selector **706a** and between the splitter **712** and the synthesis unit selector **706b**. The synthesis unit selector **706a** and **706b** then supplies the amount of active product received from splitter **712** to the appropriate module and cassette combination within the minicell **708**. Although a single box is shown for the minicell **708**, the minicell may represent multiple minicells or components provided in different room and having different production areas. Thus, the synthesis unit selectors **706a** and **706b** may supply active product to separate locations. The system **700** may also include rinse and gas supply lines **714**, as further described in connection with aspects of a splitter.

#### Process Flow Charts and Schematics

[0077] Process maps for producing example radiopharmaceutical synthesis products are illustrated in FIGS. **8-11**. These maps describe one or more of the steps and details that define each process For FDG, F-18 Product 1A, FLT, F-Miso,

F-18 Product 2, F-18 Product 1B, and F-18 Product 3. Cassette schematics are illustrated in FIGS. **30-44** corresponding to the process maps. FIGS. **9** and **11** provide a list of fluid volumes at each step to accompany the cassette schematics for an FDG example and an F-18 Product 1A.

[0078] Common process fluids, such as water, acetonitrile, and ethanol, which appear in many places in the process maps and/or may be used in multiple different processes, may be provided as bulk utilities to each module, as illustrated in FIG. **2**. In contrast, reagents, for example, which often have different concentrations of solutes in different process steps, may be packaged in a disposable reagent pack that is attached to the disposable synthesis cassette. In one variation, fluids that could mix with the process fluids during synthesis may also originate in the reagent pack, for example, to simplify quality assurance.

[0079] The cassette schematics and volume tables for the provided examples of the FDG and Example F-18 Product 1A processes, may be mapped onto example cassette schematic designs. The lists of fluid volumes incorporate a scaling down of each process to use  $\frac{1}{4}$  of the volume of fluid currently used at each step. This approach may be used, for example, to size the reaction vessel and mixing chambers. The volumes required, and other process details, may be adjusted depending on circumstances.

[0080] FIG. 8 shows an example FDG schematic **800** using isolation valves around a reaction vessel and pressure pumping for fluid transfer, in accordance with aspects presented herein. Schematic **800** illustrates components comprised in the synthesis unit **115**, e.g., mini cell **203**. In the schematic, active product **802**, e.g.,  $^{18}\text{F}$  in water is supplied to a first compartment **804**. The active product **802** may be received from a cyclotron or splitter, as illustrated in FIG. **1**. Additional materials, e.g.,  $\text{N}_2$ , water, and eluent **806**, may be added to the active product **802** in the first compartment **804**, and the combined material is thereafter supplied to a reaction vessel **806**. A first sensor **808a** may measure the activity and/or volume of the material in the first compartment. At the exit of the first compartment **804**, a supply line may be provided to the reaction vessel, and a second line **812** may lead to a fluid trap **814** for recycling at least part of the fluid, e.g.,  $\text{H}_2^{18}\text{O}$ .

[0081] An isolation valve **816a** may be provided between the exit of the first compartment and the fluid trap, and another isolation valve **816b** may be provided between the reaction vessel **806** and the first compartment **804**. Reaction vessel **806** may comprise connections to receive additional materials, e.g.,  $\text{N}_2$ , water, ACN, and a precursor and to connect to a vacuum for waste **818**. Each of these connections may comprise an isolation valve **816c-h**. A second sensor **808b** may also be provided at reaction vessel for measuring activity and/or volume. The material exits the reaction vessel and is supplied to a mixing chamber **818**. Mixing chamber may have additional connections, e.g., to receive water and  $\text{N}_2$ , and a vacuum. The mixing chamber may enable post mixing for dilution or hydrolysis. The material may be provided from the mixing chamber **818** to a fourth compartment **820**. The fourth compartment may include connections to receive additional material, a vacuum, and to distribute waste. A third sensor **808c** may be provided to measure activity and/or volume for the fourth compartment **820**. The material may be supplied from the fourth compartment **820** to a neutralizing chamber **822**. The neutralizing chamber **822** may include connections to receive additional material, and a vacuum. The material may be supplied from the neutralizing chamber through addi-



tional compartments **824** and **826** or filters **828**. The end product is then supplied to a final collection chamber **830**. Final collection chamber may comprise connections to receive additional material, to a vacuum, and to a waste line. The final collection chamber **830** then supplies the final product to a vial filler, e.g. **130**, **217**, **400**, and **500**. The compartments and lines illustrated in schematic **800** are comprised in the cassette or module within the synthesis unit.

**[0082]** FIG. 9 shows an example FDG process chart corresponding to the schematic in FIG. 8, in accordance with aspects presented herein.

**[0083]** FIG. 10 shows the Example F-18 Product 1A process schematic **1000** using isolation valves **1002 a-1**, e.g., around a reaction vessel and pressure pumping for fluid transfer, in accordance with aspects presented herein. The schematic illustrates a first compartment **1004**, a reaction vessel **1006**, a third compartment **1008**, a dilution chamber **1010**, a mixing chamber **1014**, a sixth compartment **1016**, and a final mixing chamber **1018**. The active product **1022** is received in the first compartment **1004**. The active product **1022** may be received from a cyclotron or splitter. The active product is combined with additional materials and transferred to the various compartments. Between the dilution chamber **1012** and the mixing chamber **1014**, the material may be transferred to an HPLC **1012** for purification. After the final mixing chamber **1018**, the final product may be supplied to a vial filler **1020**. Any of a first sensor **1024a**, second sensor **1024b**, third sensor **1024c**, and fourth **1024d** may be provided at the first compartment **1004**, reaction vessel **1006**, third compartment **1008**, and sixth compartment **1016**, respectively, in order to measure activity and/or volume at those locations. As described in more detail in connection with FIG. 8, each of the compartments or vessels may comprise additional connections for receiving additional materials or a vacuum connection, or for disposing of waste material.

**[0084]** FIG. 11 shows an example process chart for Example F-18 Product 1A corresponding to the schematic in FIG. 10, in accordance with aspects presented herein.

#### Cyclotron Increased Production Process

**[0085]** Aspects presented herein include methods and systems for enhanced generation of a radionuclide, such as F-18, on demand, as shown in FIG. 12. F-18 has a half-life of approximately 110 minutes, which is beneficial in that it does not pose a long-term environmental or health hazard. For example, after 24 hours, the radioactivity level is approximately 0.01% of the product when freshly produced in a cyclotron. Consequently, transport time from the production source to clinical use should be minimized to retain a maximum potency for accurate diagnostic value.

**[0086]** Conventionally, F-18 radionuclide is prepared in batches by radiating O-18 with protons from a cyclotron. Each batch must be synthesized with a pharmaceutical chemical that is preferentially absorbed by tumors. For example, F-18 FDG is a glucose-like molecule that is preferentially absorbed in tissue with high metabolic activity, which is common for some types of tumors. The radionuclide, when synthesized with a carrier molecule, may be diluted, subdivided and distributed to containers of specific volume, and therefore, of specific activity for infusion to a patient, where enhanced absorption in certain tissue, especially tumors, enables PET imaging.

**[0087]** The synthesis of a radiopharmaceutical such as F-18 FDG begins with a supply of O-18 rich water ( $\text{H}_2^{18}\text{O}$ ).

Because O-18 occurs with a natural abundance of approximately 0.2%, a concentrated supply of O-18 rich water (as  $\text{H}_2^{18}\text{O}$ ) may be costly. Currently 10 g of 98%  $\text{H}_2^{18}\text{O}$  may cost on the order of \$400-\$500. Therefore, efficient use of  $\text{H}_2^{18}\text{O}$  to synthesize F-18 FDG, and timely supply for diagnostic use once the radionuclide is created is both a cost and time driven process.

**[0088]** Some tumors, such as prostatic tumors, are much less active, and therefore a glucose-like radiopharmaceutical is not as selectively absorbed. In that case, C-11 acetate is a radiopharmaceutical that is preferably used to image evidence of prostate cancer. However, C-11 has a half-life of 20 minutes, which requires a diagnostic imaging system to be closely co-located with a cyclotron to quickly deliver the synthesized radiopharmaceutical to the patient with sufficient efficacy. It is not uncommon for C-11 to decay by several half-lives before diagnostic application for imaging. Therefore, timing is an even more critical element in production.

**[0089]** There is a need, therefore, for a method and apparatus to timely generate and deliver a radionuclide as needed, rather than to provide it from prepared batches which lose efficacy with batch storage for delayed application.

**[0090]** The on-demand system illustrated in FIG. 12 addresses these needs by providing a system for continuous production of a radionuclide on demand. This system and related methods include a pump and a first check valve to control delivery of a metered amount of a fluid containing O-18 atoms to a target cell irradiated by a proton beam, wherein the proton beam converts O-18 to radioactive F-18. A second check valve may be coupled to the target cell to control continuous removal of a portion of the solution enriched with F-18. A gas pressurized switching valve chases the portion of the solution enriched with F-18 from the system.

**[0091]** FIG. 12 shows a schematic illustration of a radionuclide continuous production system **1200** capable of producing an amount of radionuclide on demand. The radionuclide, may then be provided to a synthesizing system to bind the radionuclide to a molecule that is preferentially absorbed in a specified tissue, such as a tumor, relative to normal tissue or other differentiated organ tissues. The exemplary case described is with respect to proton conversion of oxygen-18 to fluorine-18 in a nuclear reaction with protons. The oxygen-18 is provided in the form of  $\text{H}_2^{18}\text{O}$ , which is bombarded in a cell with protons from a cyclotron having several MeV energy. However, the system **1200** may be adapted to generate other radionuclides, where the source nucleus for conversion, bombarding particle and carrier solution transporting the source nucleus may be chosen appropriately.

**[0092]** In an aspect of the disclosure, the production system **1200** illustrated in FIG. 12 may include a storage vessel **1205** that contains a quantity of O-18 in the form of stored  $\text{H}_2^{18}\text{O}$  **110**. The vessel **1205** may include a low positive pressure level of He gas to maintain a non-reactive environment in the vessel, and further to pressurize the  $\text{H}_2^{18}\text{O}$  **1210** through a transfer line **1211**. A metering pump **1215** may draw  $\text{H}_2^{18}\text{O}$  from the storage vessel **1205** through the transfer line **1211** at a selected rate, or to maintain a line pressure of, for example, 100 psi downstream. A check valve **1220** coupled to the metering pump **1215** via a transfer line **1216** maintains pressure in the lines, e.g., at 100 psi, opening to continue transfer of  $\text{H}_2^{18}\text{O}$  to a target cell **1230** contained in a target housing **1225** via a transfer line **1221** when the line pressure is sufficient. The target cell **1230** may be on the order of 1-5 ml in



volume, thereby enabling irradiation of a small volume of  $\text{H}_2^{18}\text{O}$  and consequent conversion of the small amount of O-18 to F-18, as determined by the volume of the target cell, to a concentration and an activity level determined by an amount of time of exposure to the proton beam.

[0093] The target cell **1230** interfaces with an evacuated tube **1245** via a foil **1250**. The foil **1250** may comprise Havar™, a heat treatable cobalt base alloy, which can provide sufficient strength to withstand the pressure differential between the target cell **1230** and the evacuated tube **1245** at elevated temperatures, is corrosion resistant and non-magnetic. In accordance with an aspect of the disclosure, Havar™ may be used as a pressure diaphragm foil **1250** to retain the  $\text{H}_2^{18}\text{O}$  in the target cell **1230**. The evacuated tube **1245** on an opposite side of the foil **1250** from the target cell may interface with a cyclotron (not shown) to introduce a beam of protons at several MeV energy. Energy losses of the proton beam in passing through the foil **1250** may be on the order of 1 MeV or more.

[0094] Because the beam energy may be on the order of 10-20 MeV, and the proton beam current may be on the order of 10-200  $\mu\text{amperes}$  or more, the power deposited in the target cell **1230** may be on the order of 100-4000 watts, or greater, which can result in heating and boiling of the  $\text{H}_2^{18}\text{O}$  within the target cell **1230**, and consequent over pressurization. An expansion chamber **1235** may be coupled to the target cell **1230** via a transfer line **1226** to relieve overpressure due to boiling expansion.

[0095] Additionally, a cooling heat exchanger **1255** may be coupled to the target housing **1225** and target cell **1230** to remove accumulated heat and maintain the target housing **1225**, target cell **1230** and foil **1250** at or below a selected temperature. The cooling heat exchanger may be a water line, where the water is chilled to absorb heat from the target housing **1225** and target cell **1230**. Alternatively, the heat exchanger may be a cooling or refrigeration system based on heat exchange other than water cooling.

[0096] A check valve **1260** following the target cell **1230** coupled to the target cell **1230** via a transfer line **1231** maintains line pressure upstream at, for example, 100 psi (cracking pressure 100 psi), and opens to permit transfer of irradiated fluid—which now contains F-18—to pass through a flow-through radiation detector **1265** via a transfer line **1261** when valve **1280** is closed and valve **1270** moves to position A. The flow through radiation detector **1265** measures a radiation activity level of the transferring fluid. By integrating the activity level over the transferred volume, it is possible to determine the accumulated activity level and total dose passing the radiation detector **1265**. A 4-way valve **1270** is normally in position B so that no fluid or gas is admitted. When the valve **1270** moves to position A when ready for delivery, the metering pump **1215** runs for so a predetermined level of F-18 activity passes the detector **1265**. The valve **1270** then moves to position C to provide for He chase gas to push an amount of F-18 enriched  $\text{H}_2^{18}\text{O}$  water through a transfer line **1271** for delivery **1285** to a separate system for synthesizing the radiopharmaceutical. The He pressure may be, for example about 80 psi, but may vary.

[0097] It may be appreciated that using the described system, the cyclotron beam may be run continuously. Different concentration levels of F-18 may be obtained by exposing the portion of  $\text{H}_2^{18}\text{O}$  in the target cell **130** for varying amounts of time. As a result, preparation of different doses of radiophar-

maceutical may begin with the irradiation process, and may require less complicated dilutions during the synthesis process.

[0098] The system may also include a reprocessing line **1290** that recycles and returns  $\text{H}_2^{18}\text{O}$  to vessel **1205** for reuse. The system may use electrochemical components to separate, clean, and pump  $\text{H}_2^{18}\text{O}$  back to the vessel **1205**.

[0099] The flow through radiation detector **1265** may use, for example, a CZT sensor, as described below.

#### CZT

[0100] FIG. **13** shows a schematic illustration of a gamma ray collimated detector **1300**. The sensor **1300** may include a cadmium zinc telluride (CdZnTe, or CZT) element **1310**, however, other solid state materials currently available or yet to be discovered may be used. CZT is a direct bandgap semiconductor and can operate in a direct-conversion (e.g., photoconductive) mode at room temperature, unlike some other materials (particularly germanium) which may require cooling, in some cases, to liquid nitrogen temperature. The relative advantages of CZT over germanium or other detectors include a high sensitivity for x-rays and gamma-rays, due to the high atomic numbers and masses of Cd and Te relative to other detector materials currently in use, and better energy resolution than scintillator detectors. A gamma ray (photon) traversing a CZT element **1310** liberates electron-hole pairs in its path. A bias voltage applied across electrodes **1315** and **1316** (not shown in FIG. **13**, but both shown in a side view in FIG. **14**) on the surface of the element **1310** causes charge to be swept to the electrodes **1315**, **1316** on the surface of the CZT (electrons toward an anode, holes toward a cathode). Wires **1325** and **1326** connect, respectively from electrodes **1315** and **1316** to a source of the applied voltage.

[0101] The sensor **1300** can function accurately as a spectroscopic gamma energy sensor, particularly when the element **1310** is CZT. However, geometric aspects may be considered. In conventional use of CZT as a gamma ray detector, the CZT element **1310** may be a thin platelet, sometimes arranged in multiples to form arrays for imaging, generally perpendicularly facing the source of gamma ray emission. Therefore, gamma rays of differing energies all traverse a detector element of substantially the same thickness. While absorption of the gamma ray may generally be less than 100% efficient, higher energy gamma rays will liberate more electron-hole pairs than lower energy gamma rays, producing a pulse of greater height. The spectrum and intensity of gamma ray energies may thus be spectroscopically determined by counting the number of pulses generated corresponding to different pulse heights.

[0102] Because higher energy photons may travel a greater distance in the CZT rod **1310** before complete absorption, it is advantageous for the CZT rod **1310** to be greater in length in a direction longitudinally (i.e., a long axis) intersecting a known source volume of radionuclide being measured. Gamma rays incident on the CZT rod off or transverse to the long axis may not be fully absorbed, and thus, the CZT rod will not be as sensitive a detector of such gamma rays as a result. Thus, elongating the CZT rod in one direction introduces a degree of collimation and directional sensitivity along the extended direction.

[0103] The absorption coefficient for 511 keV gamma ray absorption in CZT is  $\mu=0.0153 \text{ cm}^2/\text{gm}$ . The absorption probability as a function of  $\mu$ , density  $\rho$  ( $=5.78 \text{ gm/cm}^3$ ) and penetration distance  $h$  is

$$P(\mu, h) = 1 - e^{-\mu \rho h}.$$



[0104] Therefore, the ratio of absorption in a 10 mm length of CZT to a 1 mm length is

$$\frac{P(\mu, 10 \text{ mm})}{P(\mu, 1 \text{ mm})} \sim 9.613.$$

That is, the directional sensitivity for gamma ray detection of CZT at 511 keV along the 10 mm length of the detector is nearly 10 times greater than in the 1 mm thick transverse direction.

[0105] Referring to FIG. 14, the sensor may be a CZT rod 1310 as just described, encased in a shielded case 1305 (e.g., tungsten) with an aperture 1320 open and directed toward the transfer line 1261 to expose the CZT rod 1310 along the long dimension of the rod 1310, while shielding the CZT rod 1310 from gamma rays incident laterally to the long dimension of the rod 1310, e.g., from directions other than along the long dimension. Therefore, the combination of shielding, aperture and extended length of the CZT detector 1300 in direction of gamma ray emission from a portion of the radionuclide sample provides a substantial directional “virtual” collimation of the CZT detector’s sensitivity to gamma rays incident from the container in a volume of radionuclide defined by the collimation and the size (e.g., diameter) of the container and the collimation of the acceptance aperture 1320 of the detector 1300. On the basis that the volume of the radionuclide “observable” by the sensor is constant from measurement to measurement, the concentration and total activity of the dose can be determined, after calibration, by the integrated volume of radionuclide that passes through the transfer line 1261. In the case of the present disclosure, by knowing the flow rate and flow aperture, one can calculate the integrated dose on an ongoing basis.

[0106] The detector 1300 may also be connected to an Analog-to-Digital (A/D) converter 1330 that separate pulses of radiation so that the relevant radiation can be identified. The A/D converter may separate the pulses into separate energy brackets based on the height of the pulse for each instance of radiation received and the CZT crystal. The A/D converter may then be connected to a processing component 1340 that identifies the amount of activity in the sample based on the amount of relevant pulses identified by the A/D converter. For example, the processing component 1340 may comprise a Field Programmable Gate Array (FPGA) having code instructions setting its state to process the information for the pulses. Using an FPGA enables faster processing speeds than software run via a processor. This enables accurate and timely processing of the pulses measured by the CZT sensor.

[0107] The use of CZT solid state detectors in accordance with aspects presented herein, among other things, may allow stable measurements over time and reduction in handling and environmental (humidity) concerns by removing the need for scintillators. Furthermore, these detector elements may be compact and therefore may be packaged in smaller housings. The stopping power of CZT is also suitable for 511 keV (typical for F-18 emissions, for example) and can withstand exposure to this radiation energy level. CZT sensors may be used in any of the splitter, synthesis modules, HPLC, Low Pressure, flash chromatography or Solid phase extraction module, and in the vial filler subsystems, for example. FIG.

15 shows an example Photostat of such an example CZT sensor in accordance with aspects presented herein.

[0108] FIG. 16 shows a conceptual circuit diagram for measuring gamma rays with the detector 1600. A charge amplifier 1630 coupled to the electrodes 1615, 1616 amplifies the charge. A pulse generator 1640 converts the sensed charge to a pulse, where the pulse height is proportional to the energy of the gamma ray. A counting circuit 1650 determines the number of pulses as a function of energy.

#### Concentration-Activity Volume Sensor

[0109] One example type of CZT sensor usable, for example, in splitter and vial filler applications in accordance with aspects presented herein is referred to interchangeably herein as a Concentration-Activity-Volume (CAV) sensor. This sensor uses a slender column with two CZT sensors (e.g., which may be collimated) to measure radioactivity, and may also be used to determine volume and concentration of fluid held in the column. In one example such method for measuring volume and concentration, two sensors are oriented in an arrangement such that one sensor is located at or near the top of a vessel containing a volume to be measured, and the other is located at or near the bottom of the container. See FIG. 17, where the elements 1300 *t* and 1300 *b*, are representative of example CZT crystals usable in a CAV sensor in accordance with aspects presented herein (the actual crystals may be a different shape and aspect ratio as shown in this figure).

[0110] In contrast with some related art devices, CAV sensors in accordance with aspects presented herein do not require a concentration sensor or an optical sensor array to measure volume. As shown in FIG. 17, when the vessel 1715 is full, the two sensors 1300 *t* and 1300 *b* will have nearly equal measurements (in the case where they are both essentially equidistant from the effective center of the radiation). In cases where the fluid volume of the vessel 1715 is less than full, the bottom sensor 1300 *b*, as shown in FIG. 17, will have a higher reading than the top sensor 1300 *t*. This differential measurement may be used to determine volume information. By removing nonlinearity and subtracting background offsets in the readings, the readings from the two sensors 1300 *t* and 1300 *b* may, for example, be divided to find the volume of the fluid in the column. The total activity may then be found, and therefore the concentration, as well. The vessel has a known inner diameter and is centered with respect to the sensors (which may be mounted accurately in a fixed fashion in the vessel shielding). The vessel, which may be plastic or glass, for example, may be slid into brackets in the shielding to provide a repeatable location. Another advantage of the CAV Sensor method is that it may be less sensitive to air bubbles than a concentration sensor of the related art (which may utilize sensed information at a small cross-section of the fluid, for example).

[0111] FIG. 17 is a conceptual illustration of an apparatus 1700 for measuring concentration, activity and content volume in a container 1715 containing a radionuclide such as F-18 in solution or a radiopharmaceutical such as F-18 in FDG using the detector 1300 and circuitry of FIGS. 13-16. The container 1715 may have known dimensions, and therefore is known to be able to hold a specified maximum volume of the radionuclide in a liquid form. A first detector 1300-*b* may be located opposite a bottom face 1725-*b* of the container 1715. Similarly, a second detector 1300-*t* may be located opposite a top face 1725-*t* of the container, and is similarly



configured to detect gamma radiation from the container **1715**. The two detectors **1300-b**, **1300-t** may be similar or substantially the same. Preferably, the two detectors are identical. Therefore a description of one sensor is sufficient. Each detector, **1300-t**, **1300-b** is coupled to a differential measurement processing system **1750**, shown in greater detail in FIG. **18**.

[0112] FIG. **18** is a block diagram describing the differential processing system **1750** coupled to the two detectors, **1300-t**, **1300-b**. Processing system **1750** includes a high voltage supply **1852** to provide the bias voltage that operates each of the detectors **1300-t**, **1300-b**. Charge output from detectors **1300-t**, **1300-b** are separately input (optionally) to signal conditioning circuitry **1852** if noise filtering or DC offset correction, or other artifact removal is warranted. Alternatively, the signals from the detectors **1300-t**, **1300-b** may be directly input to a dual channel analog-to-digital converter (ADC) **1856** for processing in digital format by a customized chip, such as a flexible programmable gate array (FPGA) **1858**. The function of the FPGA **1858** will be discussed further below. Output of the FPGA **1858** includes at least computed values for the activity sensed by each of the detectors **1300-t**, **1300-b** and the volume of radionuclide in liquid accumulated in the container **1715**. The output of the FPGA **1858** may be communicated to a computing platform, such as a personal computer (PC) **1860**, or other computing controller for purposes of controlling such processes as filling or emptying the container **1715** and identifying parameters associated with the pharmaceutical content for documentation (e.g., date, activity, volume content, labeling, etc.).

[0113] The processing system **1750** may be distributed across a network to facilitate, for example, efficient use of computing resources to serve a plurality of detectors **1300** and containers **1715**. The division of the processing system **1750** across the network may be selected at any of several points. For example, one or more access nodes (not shown) and network links (not shown) may be placed between the dual channel analog-to-digital converter (ADC) **1856** and the FPGA **1858**, in which case the FPGA **1858** and the computing platform PC **1860** may be remotely located across the network. Alternatively, the access nodes and network links may be located between the FPGA **1858** and the PC **1860**. It should be understood that other network linking arrangements between the detectors **1300** and computing and control resources may be configured. The PC **1860** may also be a network configured computing resource, which may also be distributed across one or more networks. For example, the computing resource PC **1860** may include a server, memory, and other accessories, also located remotely from each other across the one or more networks to provide the operational control of the plurality of detectors **1300** coupled to respective containers **1715**.

[0114] FIG. **19** is a flowchart **1900** describing the functions of components of the FPGA **1858**. Digitized data from each channel (i.e., top and bottom) of the ADC **1856** is input to respective counters for pulse counting (process block **1902**). In conjunction with a clocking signal from a timing source (not shown) the pulse counts per unit of time (e.g., seconds) are converted to respective count rates (process block **1904**).

[0115] The count rates are then linearized (in process block **1906** for each respective detector **1300-t**, **1300-b**). The linearization process may include statistical or calibration-based correction, for example, when the count rate becomes so high that pulses may overlap, an effect referred to as "pile up."

[0116] The measured count rate, as counted by the detector and associated electronics, will become lower than the true count rate at high count rates. This is caused by effects in the bias circuitry, crystal, and the electronics. In the bias circuitry and crystal, a high photon flux can cause a shift in the spectral response (as a decreased photopeak to background ratio) which can cause undercounting. Also, the pulse width (governed by the crystal and preamplifier characteristics) along with the pulse counting electronics can have an impact on linearity. At high count rates, pulses can pile up and double or triple pulses may be combined and counted as one instead of two or three separate pulses respectively. This is exacerbated when the pulse width is increased or the counting electronics is too slow to count fast pulse rates (long retrigger times, etc.).

[0117] To linearize the count rate, a nonlinearity calibration is performed, along with implementing a look-up table or nonlinearity correction equation. To perform calibration, a high activity sample (e.g., having a maximum expected activity) is placed in front of each sensor and allowed to decay. Data is then collected over several half-lives until the count rate is low (i.e., in the linear range where no pulse pile up occurs). Curve fitting is then performed (e.g., polynomial, Lambert-W, etc.) to describe the relationship between true count rate and the measured count rate. Once established, the curve for each sensor (detector and electronics) can be used in a look-up table or equation-based correction to linearize measurements made.

[0118] Accordingly, a correction may be applied on a calibration basis to correct for an undercounting of pulses due to pulse overlap. If a background count has been detected (such as, for example, before the container is filled), a command may be issued for each detector rate to read the background rate (in process blocks **1908-t**, **1908-b**, whether from a look-up table, a previous reading from the detectors prior to filling the container, etc.). The background rates are subtracted (in process blocks **1910-t** and **1910-b**) from the respective linearized count rates.

[0119] The ratio of the resulting "adjusted" counting rates is computed (in process block **1912**) and the logarithm of the ratio is computed (in process block **1913**) which, as it happens is approximately linear in proportion to the fill level of the container **1715**. In one embodiment, the log ratio measurement may be referred to a lookup table to compute the fill volume of the container (as in process block **1914**). The fill volume depends on a known value of the shape, cross-section and height of the container **1715**. The adjusted count rate for each detector is compared with the computed volume to determine the lookup activity (in process blocks **1916-t** and **1916-b**) for each respective detector **1300-t**, **1300-b**. The outputs to the PC **1860** include the top activity level, bottom activity level, and container volume.

[0120] FIG. **20** illustrates another example sensor that may be used to measure activity. FIG. **20** illustrates a system **2000** having a cavity **2002** into which a vessel **2004** is received in order to measure the activity of material **2004** within the vessel. As with the other sensors, this sensor may be provided in connection with any of a splitter, a synthesis unit, a vial filler, a quality control component, and other components described herein. The cavity **2002** may be a lead shield, such as a pig having a 1" wall. A probe **2010** is placed adjacent the cavity **2002** and is configured to measure the activity of the material within the cavity. A spacer **2008** may be provided within the cavity in order to maintain the vessel **2004** at an appropriate height relative to probe **2010**. Probe **2010** may



comprise a CAT type sensor, as described above. Probe **2010** may comprise a diode detector, such as a pin diode detector placed at the side of vessel **2004**.

[0121] FIGS. **21a-c** illustrate a system **2100** for measuring both activity and volume of a sample **2106** within vessel **2104**. The system includes a shield **2102** that surrounds a vessel **2104**, similar to that illustrated in FIG. **20**. In both FIG. **20** and FIG. **21**, the vessel may be physically isolated from the shield. A sensor **2110** is provided adjacent to the shield, e.g., at a side of vessel **2104** in order to measure the activity of the material **2106** within the vessel **2104**. The sensor may be similar to that described in connection with FIG. **20**. Additionally, the system enables a volume measurement of material **2106** in a vessel **2104** via strain gauge **2112** or similar equipment. The shield comprises an opening into which the vessel is received. The vessel may comprise an easy extraction vial having a tapered portion **2107**. The opening **2103** extends through the bottom of the shield **2102**, as illustrated in FIG. **21b** such that the vessel can extend through the bottom opening in order to contact strain gauge **2112**. FIG. **21c** illustrates a cross section of the system, illustrating the opening **2103** in shield **2102** that enables the vessel **2104** to contact a sensor **2114** comprised in strain gauge **2112**. The vessel rests on the strain gauge sensor **2114**. A processor **2116** may interpret the measured strain in order to interpret a weight of the vessel **2104**. As the vessel fills, the strain will increase, and the strain gauge will determine the corresponding increase in volume of the material **2106** within the vessel **2104**. This system **2100** enables the activity to be measured via sensor **2110** at the same time that the volume is measured via strain gauge **2112**.

[0122] Another way in which volume may be measured is to provide a metering pump, such as a stepper motor controlled pump. This type of pump enables a known volume to be measured per predetermined number of pumps. Thus, based on the number of pumps applied, the corresponding volume may be determined.

#### Drying Process and Subsystem

[0123] Aspects of the present relation relate to methods and compositions for drying radioisotope solutions and for reducing synthesizing time of radioisotopes. The solution exiting the cyclotron may include a small fraction by volume of radioisotope (e.g., about 1% by volume) and a large fraction of O-18 enriched water (e.g., 99% by volume).

[0124] An aspect includes a method of drying a radioisotope solution having radioisotopes, the method including: 1) passing the radioisotope solution through a solid phase extraction column containing an anion exchange group, thereby trapping the radioisotopes in the column; and 2) passing an eluent through the column, thereby removing the radioisotopes from the column, wherein the eluent includes a cation trapping molecule and less than 5% water.

[0125] Another aspect includes an eluent composition for drying a radioisotope solution having radioisotopes, the composition including of a cation trapping molecule, a salt, less than 5% water, and the remainder solvent.

[0126] Additional steps for further increasing the water removal may include flushing the column with an organic solvent before passing the eluent through the column, and/or flushing the column with a high pressure inert dry gas after the organic solvent flush, but before passing the eluent through the column.

[0127] In one example implementation in accordance with aspects presented herein, the radioisotope is F-18, the extraction column is a quaternary methylammonium (QMA) column, the cation trapping molecule is 10-diaza-4,7,13,16,21,24-hexaoxabicyclo[8.8.8]hexacosane (Kryptofix 222), the salt is potassium carbonate  $K_2CO_3$ , the solvent is acetonitrile, and the water content is less than 1%. The organic solvent in the additional step is acetonitrile and the dry gas in the additional step is nitrogen.

#### Alternative Deprotection Method and Subsystem

[0128] Aspects presented herein include methods and systems for deprotecting labeled compounds, such as halogenated radiopharmaceuticals. One aspect relates to such a method (and a corresponding system for carrying out this method) comprising the steps of: 1) labeling a protected precursor compound with a labeling agent to form a labeled protected compound; 2) contacting the labeled protected compound with a solid support; 3) removing the labeled protected compound from the solid support with a removing agent; and 4) deprotecting the labeled protected compound with a deprotecting agent to form a labeled deprotected compound (final labeled compound).

[0129] Another aspect relates to a method (and corresponding system to this method) comprising the steps of 1) labeling a protected precursor compound with a labeling agent to form a labeled protected compound; 2) contacting the labeled protected compound with a medium containing two or more pieces of solid support; 3) deprotecting the labeled protected compound in the medium with a deprotecting agent to form a labeled deprotected compound; and 4) removing the labeled deprotected compound (final labeled compound) from the solid support with a removing agent.

#### Splitter

[0130] In one example implementation of a system in accordance with aspects presented herein, the splitter is the subsystem that accepts the radioactive output from the cyclotron, determines the fluid volume, total activity, and radioactive concentration of the fluid and then divides the fluid into smaller batches and sends these batches to individual synthesis cassettes. In one example implementation, the splitter has the following characteristics: accepts between 1.5 and 15 ml fluid from one or two cyclotrons; provides filtering for the fluid as it enters the splitter; determines the total activity level of the batch, for activity levels up to 30 Ci; determines the fluid volume of the batch; determines the radioactive concentration of the fluid in the batch; communicates this information to the Blackbird computer system; accepts requests from the control or other computer system for batch sizes and delivery sequence for batches to be delivered to individual synthesis units (the delivery sequence may include between 1 and 24 synthesis units); meters and delivers the batches to individual synthesis units in the sequence requested; and provides for periodic replacement of the fluid lines and the fluid storage vessel.

[0131] Additional features and operational procedures may also be included such as: any excess or left over radioactive material in the splitter vessel may be routed to the O-18 recovery tank; periodically, e.g., once per day, the splitter accumulator vessel may be rinsed with acetonitrile and then dried by flowing a dry inert gas through the vessel; periodically, e.g., once per month, the accumulator vessel and the



line sets from the splitter to the synthesis cassettes may be replaced; and periodically, e.g., every two months, the line set between the cyclotron and the splitter may be replaced.

[0132] FIG. 22 illustrates an example diagram of a splitter 2200. Splitter 2200 comprises a vessel 2202 with a line 2204 that receives active product 2205 from a radionuclide generator such as a cyclotron (not shown). The splitter 2200 may comprise a sensor for measuring activity and/or volume of the active material 2205 received within vessel 2202, e.g., sensor 2206a, 2206b. Vessel 2202 also comprises a connection 2208 to a pump 2210 for pumping the active product to a synthesis unit (not shown). A prime loop 2212 may be provided that forms a loop between the vessel 2202 and the pump 2210. The prime loop 2212 enables the pump 2210 to be primed so that an accurate amount of active product 2205 can be distributed to the synthesis unit. A meter 2214 may be provided in the line connecting the vessel 2202 to the pump 2210 in order to verify the amount of active product 2205 being pumped. The meter may comprise a step motor controlled pump meter. A rinse fluid source 2216 and a gas source 2218 may also be connected to the pump 2210 via line 2224. Valves 2226a and 2226b may be provided between this line 2224 and the rinse fluid source 2216 and the gas source 2218.

[0133] The pump 2210 may comprise a two position pump. In a first position, as illustrated in FIG. 22, the pump connects the prime loop 2212 and connects the rinse fluid 2216 and gas source 2218 to a line 2220 between the pump 2210 and the synthesis unit. This connection occurs via connectors 2222a-c. In a second position, the pump connects a supply line 2208 from the vessel to the line 2220 between the pump and the synthesis unit and connects the rinse fluid source 2216 and the gas source 2218 to a secondary line 2228 of the prime loop that leads from the pump 2210 returning to the vessel 2202. A synthesis box selector 2230 is also illustrated because a plurality of modules and cassettes, each of which can be used separately in the production of a radiopharmaceutical product. Thus, the synthesis box selector 2230 is illustrated having a plurality of lines 2232 extending to each of the plurality of module and cassette combinations and to a waste compartment 2234.

[0134] The rinse fluid may be used to alternately rinse the secondary line 2228 of the prime loop 2212 and the line 2220 leading to the synthesis box selector 2230 in order to avoid contamination. As small amounts of active material 2205 may be supplied to the synthesis box selector 2230, and accuracy is very important, the gas source 2218 may be used to send a gas bubble that moves the amount of active product 2205 from the primed pump 2210 through the line 2220 to the synthesis box selector 2230.

[0135] Although the synthesis box selector 2230 is illustrated as the intended source, the splitter 2200 illustrated in FIG. 22 may be used to distribute material stored in the vessel to other locations in the lab other than synthesis units. As an example FIG. 22 illustrates that the material stored in the vessel 2202 may be provided to a waste compartment 2234.

[0136] Aspects of splitter implementation may also vary. In one example variation, the splitter subsystem may also provide a drying function, to remove water, including the O-18 water, from the fluid before it is metered to individual synthesis cassettes. The drying function is removed from the splitter subsystem in some variations, depending on considerations surrounding the need to provide different chemistries for different product types.

[0137] The splitter may contain and then distribute the full radioactive output of one or two cyclotron targets, up to a projected future activity level of 30 Ci, hence heavy shielding (more than 3 inches of lead) may be required for some implementations. In one example variation, the splitter is located at or very near the mini-cells. For example, the splitter subassembly may be located directly on top of a mini-cell. This approach provides several advantages, including the use of the mini-cell as the shielding for one side of the subsystem and the option to route the outlet lines from the splitter directly into one or more of the shielded mini-cells. The location on top of a mini-cell has advantages over mounting locations on the side or back of a mini-cell, but both top and side mounting versions may be used in some variations, such as where a lack of clearance space exists above the mini-cells. Side mounting may possibly involve floor supported side mounting, for example, since the splitter and its required radiation shielding typically are quite heavy.

[0138] One of the functions of the splitter subsystem may be to obtain the radioactivity level of the batch as received from the cyclotron and to determine the volume of the fluid. In one variation, the system may provide this information by placing radiation sensors in accordance with aspects presented hereinabove and below the receiver vessel. One example such sensor is a CAV sensor in accordance with aspects presented herein.

[0139] One example approach provides the splitting and metering functions via a positive displacement pump that is controlled to sequentially pump the requested volume for an individual batch through a selector valve to one of 12 lines, for example, per the system computer's requests. The pump option selection may be based, for example, on considerations of range of flow rates available and volumetric flow accuracy. After the pump pushes the desired fluid volume into the line, the fluid may be moved to the selected synthesis module by a bolus of inert gas injected behind the fluid, for example. The pump and selector valve may then be ready to deliver the requested volume of fluid to the next synthesis unit in the requested sequence.

[0140] An overview of an example splitter, e.g., 110 from FIG. 1, subsystem in accordance with aspects presented herein is shown in FIG. 23. In FIG. 23, because the splitter system 2300 may contain and distribute the radioactive output of one or more cyclotron targets, for example, up to a projected future activity level of 30 Ci, the system 2300 may be provided with a heavy shielding enclosure 2340, composed for example of three inches of lead. The shielding enclosure 2340 may include one or more access means 2344, such as a hinged door or panel, to provide easy and efficient access to the shielded components for removal, replacement, and/or maintenance. For example, the fluid vessel 2202, fluid delivery lines 2204, 2208, 2220, 2224, and 2228 160, fluid evacuation tubes may be replaced periodically, such as once per month.

[0141] FIG. 24 illustrates an exemplary splitter system 2410 that may incorporate a CAV sensor assembly 2430, a pump 2450, and a selector valve assembly 2460. The CAV sensor may include a fluid vessel 2410 positioned in a CAV enclosure 2420. The CAV sensor assembly 2430 is an apparatus for measuring various properties of a liquid radionuclide material.

[0142] The CAV sensor assembly 2430 may determine the volume, activity and activity concentration of the product received into the fluid vessel 2410. The information from the



CAV sensor assembly **2430** may be automatically provided to a control system **150**, or the information may be read from the CAV sensor assembly **2430** by a technician, for example, and manually input into the control system **150**. The CAV sensor assembly **2430** may determine the activity concentration, activity, and/or volume components of the radioactive product delivered to the fluid vessel **2410**. Once the desired parameters have been measured by the CAV sensor assembly **2430**, the pump **2450** may be used to draw discrete volumes of the radioactive product from the fluid vessel **2410** to deliver a desired activity.

[0143] The CAV enclosure **2420** may be configured to ensure that the fluid vessel **2410** maintains a proper alignment with radiation sensors, which may be used to determine specific properties of a radioactive product delivered into the fluid vessel **2410**, such as, for example, a fluid volume, total radioactive activity, and a radioactive concentration of the product.

[0144] The splitter system **2400** may receive the radioactive product directly from one or more generation sources, such as a cyclotron(s), for example. A fluid delivery tube may be configured to deliver the radioactive product from the generation source to the fluid vessel **2410**. The fluid delivery tube may be configured to pass through a wall of the CAV enclosure.

[0145] In accordance with another aspect of the present invention, as shown more particularly in FIG. **24**, an inlet/outlet cap **2470** may be provided to mount on the fluid vessel **2410**. The inlet/outlet cap **2470** may be connected to the fluid delivery tube **2460** to permit delivery of the radioactive product into the fluid vessel **2410**. Simultaneously, a separate fluid evacuation tube **2480** may be connected to the inlet/outlet cap **2470** to permit evacuation of the radioactive product from the fluid vessel **2410**. The radioactive product may be pumped out of the fluid vessel **2410** via the fluid evacuation tube **2480** by the pump **2450**.

[0146] As shown in FIGS. **25A** and **25B**, the pump **2450** may be a positive displacement pump controlled to pump a requested volume of the radiopharmaceutical product. The pump **2450** may have a body **2510** with an inlet port **2512** and an outlet port **2514** and operated, for example, by a solenoid **2520** connected to the body **2510**. Lead wires **2524** may be configured for connecting the pump **2450** to a power source. The pump **2450** may be a self-priming micro-pump, for example, capable of dispensing discrete volumes of the radiopharmaceutical product, such as volumes between 10-60  $\mu$ l. Check valves (not shown) may be situated at the inlet port **2512** and outlet port **2514** to control the direction of flow. In addition, a diaphragm (not shown) may be provided to isolate the operating mechanism from the flow path between the inlet port **2512** and the outlet port **2514**.

[0147] As shown in FIG. **25B**, the body **2510** may be provided with mounting holes **2530** for mounting the pump **2450** at a location most suitable for operation and/or maintenance. For example, as shown in FIGS. **22-27**, the pump **2450** may be mounted to a pump bracket **2440** via the mounting holes **2530** to be situated in the vicinity of the rear of the enclosure **2420**.

[0148] The pump **2450** may be controlled by a control system **2880** to sequentially pump a requested volume for each individual batch from the fluid vessel **2410**, through the evacuation tube **2480**, and to the selector valve assembly **2602** via a pump delivery tube **2760**. The evacuation tube **2480** is connected to the inlet port **2512** of the pump **2450** and

the pump delivery tube **2760** is connected to the outlet port **2514** of the pump **2450**. In accordance with yet other aspects presented herein, a fluid flow meter (not shown) and/or filter assembly (not shown) may be provided between the CAV sensor assembly **2610** and the pump **2450** and/or between the pump **2450** and the selector valve assembly **2602**.

[0149] As shown in FIGS. **26** and **27**, the selector valve assembly **2602** may include a selector valve **2620** actuated by an actuator **2490**, which, for example, may be an electric or pneumatic actuator. The pump delivery tube **2760** provides fluid communication between the pump and an interior chamber of the selector valve **2620**. The radioactive product is provided to the CAV sensor assembly **2610** via the fluid delivery tube **2660**. The selector valve **2620** may be actuated to send a volume of the radioactive product from the fluid vessel **2410** to any one of as many as twelve lines for delivery to a synthesis unit (not shown).

[0150] The splitting and metering functions of the pump **2450** and selector valve assembly **2602** are controlled by the control system to sequentially pump the requested volume for an individual batch through the selector valve **2620** to one of the lines. After the pump **2450** pushes the desired fluid volume into the selected line, the fluid volume is moved to the selected synthesis module by a bolus of inert gas injected behind the fluid. The pump **2450** and selector valve **2620** are then ready to deliver the next requested volume of fluid to the next synthesis unit in the requested sequence.

[0151] In accordance with other aspects of the present invention, more than one selector valve assembly **2602** may be provided, if more than twelve lines **2785** are desired for selective delivery of product to additional synthesis units. For example, if the splitter system **2604** is configured with a second selector valve assembly **2602**, a 2-way selector valve would be added and the control system configured to direct the pump **2450** output to the desired selector valve assembly **2602**.

[0152] In accordance with yet other aspects of the present invention, as shown in FIGS. **22-27**, the CAV sensor assembly **2610**, pump **2450**, and the selector valve assembly **2602** may be mounted to a mounting platform **2606**. For example, the CAV sensor assembly **2610** may be mounted to the mounting platform **2606** via the CAV enclosure **2420**, the pump **2450** via the pump bracket **2440**, and the selector valve assembly **2602** via a selector valve bracket **2680**.

[0153] For example, the pump may comprise a BIO-CHEM Micro-Pump 120 SP Series. The synthesis unit selector may comprise a VALCO A3CSD12MWE 12-Position Flowpath Selector, and the splitter may further comprise a pneumatic actuator such as a VICI A123 Air Actuator.

[0154] As shown in FIG. **3**, the splitter system **310** may be incorporated into a system that includes a mini-cell assembly **300**. Because of the weight of the shielding enclosure for the minicell, the splitter system may be provided directly on an upper surface of the mini-cell assembly **300**. Because the mini-cell assembly **300** is also shielded, one side of the shielding enclosure for the splitter **310**, such as the lower side, may be shielded via the shielding of the mini-cell assembly **300**. In addition, the outlet lines of the splitter system may be routed directly into the shielded mini-cell assembly **300**. If a lack of clearance above the mini-cell assembly necessitates a location of the splitter system to a side or rear of the mini-cell assembly, a floor support structure (not shown) may be required to support the heavy load of the splitter system **310** due to radiation shielding.



[0155] FIG. 28 is a functional flow diagram of the splitter system 110. Production of a radioisotope, such as fluorine-18, for use in the radiopharmaceutical occurs via the cyclotron (not shown), and the radioactive product is provided to the CAV sensor assembly 2810 via the fluid delivery tube 2860. The CAV sensor assembly 2810 determines certain product properties, such as the liquid volume and activity level of the delivered product and activity concentration, and provides the information to the control system 2880 so that the required volume required to achieve a desired activity for delivery to a specific location (e.g., a synthesis module) can be computed and drawn. Accordingly, the control system 2880, in response to inputs from a user, for example, subsequently calculates the required volume of the product to be delivered to a specific location, such as a specific synthesis unit in the mini-cell assembly 2820. The pump 2850 is controlled to pull the required volume for delivery to the required location via the selector valve assembly 2830. A flow sensor 2890 may be provided to record the volume delivered to the pump 2850. The control system 2880 provides a signal to the selector valve assembly 2830 to actuate the valve selector to open communication through one of the lines 2870 in accordance with the required location. A purge signal may be sent from the control system 2880 to provide a volume of purge gas, such as nitrogen, to clear the lines and force the radioactive product out of the line 2870 into the required location. The control system 2880 may then perform the above sequence until each of the required volumes is delivered to each of the required locations.

[0156] The subsystem illustrated in FIG. 23 may include one 12-way selector valve, for example. This arrangement is suitable, for example, for an installation with a dual mini-cell configuration (two mini-cells containing up to six synthesis modules each). For installations with four mini-cells, another 12-way selector valve may be installed, and a 2-way selector may be added to direct the pump output to the desired 12-way selector.

[0157] The splitter subsystem may optionally incorporate panels that may be removed to provide access to the fluid vessel and the fluid lines for periodic replacement. The fluid vessel may be positioned in a fixture that maintains proper alignment with the radiation sensors after vessel replacement, for example.

#### User Interface

[0158] FIG. 29 illustrates an example user interface 2900 for entering instructions into the system. The user interface may be provided at the location of the splitter 110 and/or minicell 115. The user interface comprises a main tab 2902 that receives a selection of a cell 2904. Once a cell is selected, the tab switches to the keypad tab 2906 that provides a keypad for receiving a type and amount of radiopharmaceutical product to be produced. The screen then returns to the main tab 2902 and is able to receive the selection of an additional cell. Once the user has finished entering instructions, the user interface is configured to start production upon receiving a start delivery command 2908. The user interface may further comprise graphics 2910 that illustrate a volume and activity amount for the active product. The user interface may further illustrate a connection 2912 between the splitter and a selected cell in order to show a user the cells currently being used. For example, a pathway may light up when active. A third tab 2914 provides options for maintenance and rinsing features.

[0159] The user interface 2900 provides visualization of the process and will graphically depict the status of the system. The user interface provides a simple graphical interface for batch operation as well as have additional screens that depict a more in depth view of the process for diagnostics and troubleshooting. The status 2916 of devices, such as the positions of valves and actuators, may be color coded for easy recognition. Process variables and alarm status may be easily accessible and viewable by the operator.

#### Valveless Pressure Pumps

[0160] Aspects presented herein include valveless pressure pump features, such as for: 1) membrane pumping (also referred to herein as reverse side pumping); and 2) cascade pumping.

#### Membrane Pumping

[0161] In applications where a fluid must be transferred between a plurality of chambers, there are typically losses of fluid that tends to remain inside valve materials, in crevices, or other geometrical features of the valve materials. In addition, in order to perform fluid transfer, relatively complex equipments including pumps and valves that take up large spaces are generally needed. Accordingly, there is a need in the art to provide systems and methods that can ensure pumping operations taking place entirely within a disposable cassette so that, for example, durable components are not contaminated by, nor contaminate, the working fluid, and to ensure fluid transfer from one chamber to the next without fluid loss.

[0162] In light of the above described problems and unmet needs, systems and methods according to aspects of the present invention provide a container with one or more fluid passageways having highly isolated and pressure-resistant valves using an actuated membrane. According to various aspects, the container may be a substantially three-dimensional container having two elongated dimensions and a thin third dimension so as to have two main faces formed by the two elongated dimensions. According to an aspect, the fluid passageways may be located closer to one side of the container, and the pressure-resistant valves may be located on an opposite side of the container from the fluid passageways. The fluid passageways and valves may be interconnected with open holes, or scoops, located throughout the container.

[0163] Aspects presented herein include a compact modular cassette system and method for the synthesis of radiopharmaceutical products that includes a modular unit having reagent modules and a reaction cassette, the reaction cassette having an actuated flexible membrane placed over valve features formed by open holes or scoops on a side of the cassette and at desired locations of the cassette. The actuated membrane may be disposed on an opposite side of the cassette from the cassette side that is in contact with other modules and that contain one or more fluidic channels and passageways. When a portion of the membrane that is located over a scoop is actuated, the membrane portion may be either urged against the scoop, or pulled away from the scoop. When the membrane portion is urged against a scoop of the fluid passageways, for example, the membrane portion may seal tightly against the scoop of the passageway, thus blocking any ingress or egress of fluid. Alternatively, when the membrane portion is urged away from the scoop of the fluid passageway, then a suction or pumping action may take place. As a result,



any fluid present in one or more passageways connected, and in proximity, to the pumping scoop may be urged inside the one or more passageways as a result of the pumping action created by the membrane portion on the pumping scoop.

[0164] Smaller open holes or scoops, to be used as valves, may be located on one or more sides of a central scoop along the path of a fluid passageway, the smaller scoops being usable as valving scoops. Accordingly, when a portion of the membrane alternatively seals against, or pulls away from, one or more of the valving scoops in conjunction with another membrane portion operating a pumping action, as discussed above on the larger pumping scoop, the direction of movement of the fluid inside the one or more passageways connected to the pumping scoop and to the one or more valving scoops may be controlled. Accordingly, fluid flow may be created, controlled and monitored using the flexible membrane being actuated over the pumping scoop and one or more valving scoops, to form a membrane pumping system. FIG. 30 contains a Photostat of an example pump detail in accordance with aspects presented herein, including “opposite side” geometry with arrows indicating flow direction. FIG. 30 is a schematic illustration of a membrane pumping system that may be used in a reaction module or cassette, according to various aspects of the current invention. In FIG. 30, the system 3000 includes a fluidic cassette 3010, which may be a reaction module, that includes a plurality of etched, molded, machined, or otherwise formed passageways 3020, formed inside the cassette 3010. The reaction cassette 3010 may be a substantially three-dimensional module with two opposite surfaces and a thin third dimension. The passageways 3020 may be formed within the module 3020 but may also open on a surface of the cassette 3010 at open holes 3030, and scoops 3040 and/or 3050, which may all have the same size, or may have different sizes. The arrows illustrated in FIG. 30 indicate the flow path of fluid inside the cassette 3010. It should be noted that the fluid passageways 3020 may be formed on only one side, or on both sides, of the cassette 3010. Although scoops 3030 may be formed on both sides of the cassette 3010, scoops 3040 and 3050 may only be open on a single side of the cassette 3010, e.g., the side that is opposite to the side where the fluid passageways 3020 are formed.

[0165] The passageways may be formed closer to one side of the cassette 3010 that may be a side opposite to a side where the scoops 3030, 3040 and 3050 are formed, and because of the location of the fluid passageways 3020, the flow path may primarily take place on the side of the cassette 3010 that is opposite to the side where the scoops 3030, 3040 and 3050 are located. The flow of fluid may be controlled via membrane pumping, as described in greater detail below, where the arrangement of a pumping scoop 3050 and one or more valving scoops 3040 on one or more sides of the pumping scoop 3050, each of the scoops being covered by a portion of the membrane, constitutes a membrane pump that is activated by applying a differential pressure on the portion of the membrane located over one or more of the scoops 3040 and 3050. For example, the portion of the membrane located over the larger pumping scoop 3050 can be urged against the scoop 3050 to seal the pumping scoop 3050 and then pulled back away from the scoop 3050, thus creating a pumping action. The one or more scoops 3040 may be used as valves to allow or deny fluid or gas from entering the fluid passageway and thus control the direction of the flow of fluid located in the cassette 3010. The one or more scoops 3040 may be connected to two fluid passageways that only communicate with

each other via the scoop 3040 and that are also connected to the main fluid passageways 3020. Accordingly, when the portion of the membrane that is above a scoop 3040 is pressed against the two passageways, flow of fluid from one passageway to the other is interrupted. As a result, the scoop 3040 may be used as a valve, as discussed in more detail below.

[0166] A plurality of such pumping arrangements can be formed on the surface of the cassette 3010, indicating the existence of a plurality of membrane pumps on one or more surfaces of the cassette 3010 that control the flow of fluid in the fluid passageways 3020. Accordingly, when the fluid passageways 3020 connect several modular cassettes, fluid transfer can be performed between the plurality of modular cassettes, where fluid is transferred from the fluid communication channels of one cassette onto fluid communication channels of another channel. It should be noted that although FIG. 30 illustrates a structure with three scoops, one central scoop 3050 that functions as a pump and two scoops 3040 that function as valves, a higher number of scoops may be configured, with various combinations of scoops functioning as pumps and scoops functioning as valves.

[0167] FIG. 31 is a schematic illustration of a plurality of scoop profiles and an actuatable flexible membrane. In FIG. 31, a membrane portion 3160 covers a portion of the surface of the cassette 3010 where the pumping scoop 3050 is located, and other membrane portions 3166 and 3168 cover other portions of the surface of the cassette 3010 where the valving scoops 3040 are located. The membrane portions 3160, 3166 and 3168 may be controlled by an actuator 3170, which may urge one or more of the membrane portions 3160, 3166 and 3168 independently of each other to seal tightly against the scoops 3040 and/or 3050, or may urge one or more of the membrane portions 3160, 3166 and 3168 independently to pull away from the scoops 3040 and/or 3050 in order to transfer the fluid through the passageways 3020.

[0168] In operation, when fluid is present in the passageways 3020, the fluid may be urged in any direction by actuating various portions of the membrane 3160 located at various locations of the surface of the cassette 3010. For example, when the membrane portion 3160 is urged against the pumping scoop 3050 of the fluid passageways 3020, the membrane portion 3160 may seal tightly against the pumping scoop 3050, and another membrane portion 3166 and/or 3168 that is located over one or more of the valving scoops 3040 may or may not be urged against either valving scoop 3040. In FIG. 31, the pumping scoop 13050 covered by a membrane portion 3160 may function as a pump, while the scoops 3040 covered by membrane portions 3166 and 3168 may function as valves.

[0169] Valving scoops 3040 may be connected to two fluid passageways 120a and 3020b, or 3020c and 3020d, as illustrated in FIG. 31. When a valving scoop 3040 is covered with the membrane portion 3168, the fluid passageways 3020a and 3020b are formed in the body of the cassette 3010, but only communicate with each other via the scoop 3040. In other words, fluid can only move from passageway 3020a to passageway 3020b, or vice-versa, via the scoop 3040. The passageways 3020a and 3020b are also connected to the main fluid passageways 3020 in order to allow fluid to move from the main passageway 3020 into the scoops 3040 and/or 3050 and back to the passageway 3020. Accordingly, when the portion of the membrane that is above a scoop 3040 is pressed tightly against the two passageways 3020a/3020b or 3020c/13020d, as illustrated by the dotted line representing the location of the membrane portion 3168 and 3166 pressed



immediately over the opening of the passageways **3020a** and **3020b**, or over passageways **3020c** and **3020d**, flow of fluid from one passageway **3020a** to the other passageway **3020b** is interrupted because the fluid can no longer travel from one passageway to the other. As a result, the scoop **3040** may operate as a valve.

[0170] Either one of the valving scoops **3040** may be either closed or open. The movement of fluid inside the passageways **3020** may be controlled via the combination of the pumping action of the membrane portion **3060** on the pumping scoop **3050** and the valving action of the valving scoops **3040**. The pumping and valving actions created by the membrane portions **3160**, **3166** and **3168**, create, control, and monitor fluid flow inside the cassette **3010**.

[0171] FIG. **32** is a schematic illustration of a reaction cassette that may be used with such a membrane pumping system. In FIG. **32**, the reaction cassette **3210** includes a fluid chamber **3250** and fluid communication channels **3220** formed inside the cassette **3210** to transfer fluid in and out of the fluid chamber **3250** during a reaction process. The fluid communication channels **3220** may also be connected to other fluid communication channels **3230** that may be part of another fluid containing chamber within the cassette **3210**, or to outside fluid communication channels. The fluid channels **3220** and **3230** may be connected to each other in order to ensure fluid transfer via one or more membrane valves **3240** that are similar to the valving scoops and membrane portion arrangements discussed above. The membrane valve **3240** may include a flexible membrane (not shown) disposed over a scoop (not shown) formed on the surface of the cassette **3210**, and may allow, or deny, passage of fluid from a fluid communication channel **3220** to another fluid communication channel **3230** according to the valving mechanism discussed above with respect to FIG. **31**.

[0172] According to various aspects, the above system and operation, such as the operation of the flexible membrane actuator, can be controlled and operated via hardware and software, as discussed in greater detail below.

#### Cascade Pumping

[0173] According to various aspects presented herein, one or more chambers may be supplied with pneumatic transfer lines or channels connecting the chambers to one another, and allowing the selective flow of pressurized gas and/or the application of a vacuum to the chambers. The channels may connect, for example, a lowest point in a first chamber to a high point in a second chamber in order to ensure that the totality of the fluid present in the first chamber is transferred to the second chamber (e.g., by gravitation). According to various aspects, in order to ensure complete transfer of fluid from a first chamber to a second chamber, a vacuum may be applied to the second chamber, which is the chamber to which the fluid is to be transferred, through, for example, a line communicating the second chamber with a vacuum source, and a flow of pressurized gas may be applied to the first chamber, which is the chamber in which the fluid is located prior to transfer, through, for example, a line communicating the first chamber with a source of pressurized gas. The application of the vacuum to the second chamber and the flow of pressurized gas to the first chamber may be performed contemporaneously. Accordingly, the combined action of the pressurized gas pushing the fluid out of the first chamber, and the vacuum pulling the fluid towards the second chamber,

may ensure a more complete and rapid transfer of the fluid from the first chamber to the second chamber.

[0174] FIG. **33** is a schematic illustration of a plurality of mixing chambers **3310**, **350** and **190**, disposed according to various aspects of the current invention. In FIG. **33**, the cavity in each chamber may be large enough to allow a two-phase mixture of liquid and vapor, and to establish a fluid level with the vapor located above the fluid. According to various aspects, each chamber may have one or more entry and exit passages. For example, the chamber **3310** may have input lines **3312** and **3314** to allow for the input of fluids, reagents and other like ingredients, where the chamber **3310** may be a reaction chamber in which various ingredients, solid, liquid, or gaseous, may be input via the input lines **3312** and **3314** and mixed or reacted together. According to various aspects, the line **3322** may be used to provide the chamber **3310** with a pressurized gas such as, for example,  $N_2$  by opening a valve at the line **3322**. It should be noted that the pressurized gas that flows in the chamber **3310** via the line **3322** may be any combination of gas or gases other than  $N_2$ , such one or more inert gas, but can also be a gas such as oxygen or air as long as the gas that does not interact with the fluid composition or ingredients present in the chamber **3310** to create an unwanted chemical reaction. It should be noted that a gas referred to as “inert” in this disclosure is inert with respect to the fluid, ingredients or reagents present in the chamber **3310**, even if the gas is not inert with respect to other compositions or other compounds.

[0175] An exemplary purpose of the pressurized gas provided via the line **3322** to the chamber **3310** is to apply a downward pressure to the fluid present in the chamber **3310** and urge the fluid out of the chamber **3310** to, for example, chamber **3350**, via the transfer line **3330**. According to various aspects, the chambers **3310**, **3350** and **3390** may be configured so as to have an amount of space, or distance, between the vacuum lines **3324**, **3364** and **3384** and the free surface of the fluid in order to prevent splashing or splattering from causing fluid to be ingested by the vacuum lines and thus to be lost from the process. For example, vacuum lines may be connected to the chambers from the top of each chamber so that the fluid and the gases in the chamber have enough space to interact without being ingested by the vacuum created in a vacuum line. According to various aspects, baffles may be used to prevent the fluid from being ingested in a vacuum line. The additional amount of space above the free surface of the fluid may also be useful when sparging the fluid to remove any gases dissolved in the fluid.

[0176] According to various aspects of the current invention, the end of the transfer line **3330** that is placed inside the chamber **3310** and which may be cut on a bias to have an opening that is non-perpendicular to the axis of the line **3330**, may be located at a lowest point of the chamber **3310** in order to ensure that all of the fluid initially located in the chamber **3310** can be transferred to the chamber **3350**. As a result, the shape of the chamber **3310** may include a lowest point and may have a conical or triangular shape, the point of the triangle or cone being the bottom of the chamber **3310**. It should be noted that although FIG. **33** illustrates transfer lines **3330** and **3370** that are located inside the chambers **3310** and **3350**, according to various aspects of the current invention, the transfer lines may also be located outside of the chambers so as to drain the contents of the chambers from an outside location, as long as the end of the transfer line is at the lowest point of the chambers. For example, a transfer line may be



configured so as to come out of a chamber, either in a vertical direction along the center axis of the chamber, or from the side of the chamber. In either configuration, the end of a transfer line may be located at the lowest point of the chamber from which fluid is being transferred. According to various aspects, the other end of the transfer line **3330** may be located at a high point of the chamber **3350**, which is a point above the fluid level of the chamber **3350**.

[0177] In order to transfer all of the fluid present in the first chamber **3310** to the second chamber **3350**, the line **3322** may be opened to allow a pressurized inert gas to flow into the chamber **3310** and to create a pressure urging the fluid downward in the chamber **3310** and ultimately out of the chamber **3310** via the transfer line **3330**. In addition, the gas line **3362** in the second chamber **3350** may be closed, and the vacuum line **3364** in the chamber **3350** may be opened by opening a vacuum valve located at the line **3364**. As a result, a vacuum is created in the chamber **3350**, and because the only other open opening in the chamber **3350** is the transfer line **3330** that is connected to the fluid in the chamber **3310**, a suction action of the fluid present in the first chamber **3310** is created through the transfer line **3330**. Accordingly, the combined action of the pushing action of the pressurized gas flowing in the chamber **3310** via the line **3322** and of the suction action of the vacuum created in the transfer line **3330** and provided via the chamber **3350** results in the entirety of the fluid present in the chamber **3310** to be transferred rapidly to the chamber **3350**. Accidental subsequent fluid transfer to chamber **3390** from chamber **3350** may also be prevented by maintaining a positive pressure inside the chamber **3390** and the transfer line **3370** by, for example, flowing gas via the gas line **3382** into the chamber **3390** and possibly in the transfer line **3370**. As a result of the existence of the positive pressure in chamber **3390**, no fluid that has been transferred from chamber **3310** to chamber **3350** can accidentally be further transferred to chamber **3390**.

[0178] It should be noted that during the transfer process, the pressurized gas line **3362** of the chamber **3350** may remain closed, and no pressurized gas is provided to the chamber **3350**. However, a pressurized gas may be provided to the chamber **3350** via the gas line **3362** before any fluid transfer from the chamber **3310** to the chamber **3350** in order to keep the fluid in the chamber **3310** and avoid accidental transfer of fluid via the line **130** before such time when fluid transfer is desired. Accordingly, the pressurized gas is flowed inside chamber **3350** via the gas line **3362** while the vacuum line **3364** is closed. Because the only other opening in the chamber **3350** is the transfer line **3330**, the pressurized gas flows through the transfer line **3330** into the fluid present in the chamber **3310**. As a result, gas sparging or bubbling of the fluid may occur at the end of the transfer line **3330** located at the bottom of the chamber **3310**, which may prevent any amount of fluid from accidentally being transferred from the chamber **3310** to the chamber **3350**. Accordingly, accidental fluid transfer may be avoided, and no fluid is transferred before fluid transfer from chamber **3310** to chamber **3350** is desired.

[0179] The chamber **3350** may also have one or more input lines such as input lines **3352** and **3354**, through which additional reagents, or ingredients, may be provided, for example during a second stage of a manufacturing or reaction process, after or before the fluid has been transferred from chamber **3310** into chamber **3350**. Accordingly, mixing of various additional ingredients with the fluid transferred from the

chamber **3310** to the chamber **3350** may take place inside the chamber **3350**. A subsequent transfer of the fluid now present in chamber **3350** to chamber **3390** can be accomplished in a similar process to the process described above with respect to the transfer of fluid between chambers **3310** and **3350**. To transfer the fluid from chamber **3350** to chamber **3390**, gas line **3362** is opened to allow flow of a pressurized inert gas into chamber **3350** while vacuum line **3384** of the chamber **3390** is opened to create a suction action. As a result, the fluid present in chamber **3350** is entirely transferred to the chamber **3390** via transfer line **3370**. In chamber **3390**, additional ingredients or reactants may be added to the fluid via input lines **3392** and **3394**.

[0180] Accordingly, an additional mixture or reaction of various fluids and chemicals may be performed in the successive chambers **3310**, **3350** and **3390** during separate successive stages of an overall chemical process, and various effluents or fluids may be transferred to one or more of the chambers by manipulating the vacuum lines and pressure lines of the various chambers as discussed above, and without having to use wet valves or pumps in the transfer lines. For example, chemical synthesis may be performed in the various chambers **3310**, **3350** and **3390** illustrated in FIG. 33. It should be noted that although only three chambers are illustrated in FIG. 33, there may be as many chambers as needed to effectuate any required number of reaction steps. It should also be noted that although the three chambers **3310**, **3350** and **3390** are illustrated as being disposed in a generally vertical direction, the chambers may be located on the same plane, or have one or more chambers be located higher or lower than the other chambers. Also, with respect to the valves used to open and close the various gas, vacuum and input lines, many types of valves may be used such as, for example, ball valves, butterfly valves, globe valves, gate valves, diaphragm valves, check valves, and the like.

#### Modular Synthesis Subsystem/Backplane

[0181] In one example implementation of a system in accordance with aspects presented herein, a modular synthesis subsystem/backplane, examples of which are also interchangeably referred to herein as Multi-Synth Units, which may include for example hardware contained in a mini-cell. One variation of the Multi-Synth incorporates up to six synthesis modules in one mini-cell. Since the synthesis modules, the HPLC modules, and the cassette/reagent pack hardware are further described elsewhere herein, the Multi-Synth discussion in this section focuses on the remaining hardware, such as the module supporting structures, the backplane hardware, and provisions for installing the hardware and making electrical and plumbing connections.

[0182] To provide maximum flexibility in some variations, the Multi-Synth unit may accommodate six modules simultaneously. For a given processing run, these six modules could be all the same type, such as FDG synthesis modules, or they could be a mixture of several types of synthesis modules, such as FDG and Example F-18 Product 1A modules, and one or two HPLC modules.

[0183] FIGS. 34-36 illustrate views of one example Multi-Synth design approach in accordance with aspects presented herein. In this approach the six modules **3402** are arranged in a 3 module **3402** wide by 2 module **3402** high configuration. This configuration provides best utilization of the example minimum interior mini-cell **3400** dimensions indicated. In



this configuration, either or both of the two modules on the right side of the Multi-Synth may be configured as HPLC modules **3404**, for example.

**[0184]** In this example, a framework supports the six modules, and this framework is attached to rack slides **3602** that permit the entire framework to be pulled forward from the mini-cell to provide access to the modules and the backplane (see FIG. **36**). The rack slides will need to be firmly attached to the mini-cell to prevent tipping as the Multi-Synth framework is pulled forward. An initial estimate of the weight of the complete Multi-Synth unit for this example, with six modules installed, is in the range of 200 to 300 lbs. Most of this weight is in the modules themselves. Safeties, such as mechanical stops to prevent overextension and positive retainers to keep the rack slides securely in place, may be provided.

**[0185]** In one example implementation, the modules are installed in the framework by sliding them in from the front on low friction ways. A retaining pin or similar device may be used to provide positive retention once installed in the framework. Since ease and speed of removing and installing modules may be useful, most or all of the connections between the module and the backplane may be made automatically or easily as the module is pushed to the back of the framework, without the need for manual and/or other complex connection of individual fluid, gas, or electrical connections.

**[0186]** Additional details of such a modular cassette synthesis unit design approach are provided in U.S. Provisional Application No. 61/508,373, titled "MODULAR CASSETTE SYNTHESIS UNIT," the entire contents of which are hereby incorporated by reference herein.

#### Cassette and Reagent Pack

**[0187]** The overall cassette and reagent pack example outlined in this section provide disposable components for synthesis systems that have advantages over the components currently used in synthesis systems of the related art. Features of the overall cassette and reagent pack may include: small and compact hardware that is compatible with the Multi-Synth approach that incorporates six synthesis modules in one mini-cell; small cassette elements that process batches with activity levels up to 30 Ci but with smaller fluid volumes than currently used in the MX system; a cassette design that reduces processing time and provides consistently high yields; a cassette/reagent pack that is simple to install and does not require manual connections; and a cassette/reagent pack design approach that is configurable such that more than one radiopharmaceutical product can be processed per cassette mold design.

**[0188]** In one example system in accordance with aspects presented herein, the cassette is the component in which the synthesis is performed. The cassette performs the functions that are primarily performed by the disposable elements used in certain related art MX synthesis units. In the initial design approach, the cassette may contain several synthesis elements, including: 1) QMA cartridge; 2) a reaction vessel; 3) heating provisions for the reaction vessel; 4) chambers for mixing, neutralizing, and final product collection; and 5) one or more solid phase exchange cartridges. In addition, the cassette may incorporate numerous passages, connections, two-way membrane valves, and membrane pumps, for example.

**[0189]** The cassette may be held in contact with the module and have pneumatic, fluid, and electrical connections contained within or attached thereto. The side of the cassette

opposite the module may be held in contact with a reagent pack, for example. The reagent pack, in one variation, has approximately the same footprint as the cassette, and may be clamped in contact with the cassette by mechanical clamping or other suitable coupling features. The reagent pack may contain the fluids and powders that are unique to the production of a specific radiopharmaceutical formulation. The reagent pack may either be a single component, or it may have one or more small insert sections, as needed, based on the storage requirements of the reagents. The reagent pack may be stored refrigerated, and an insert section could be stored separately if other requirements, such as freezing, are needed, for example.

**[0190]** FIGS. **37** and **38** show views of an example variation of an FDG cassette and reagent pack installed on an example module, in accordance with aspects presented herein.

**[0191]** Further to as described in the Multi-Synth section hereof, in one variation, six modules are incorporated in a three wide by two high configuration in one Multi-Synth unit. FIGS. **34-36** show example views of one such arrangement configured with six synthesis modules. Each of these modules can support a synthesis cassette/reagent pack disposable subsystem. Based on space constraints in the mini-cells in this example, the modules each have approximately an 8" by 8" cross section, and an overall depth of about 10".

**[0192]** Since there may be more than one cassette configuration needed to accommodate the range of radiopharmaceutical products, more than one module configuration may be used. For example, one module configuration may be used for FDG and similar products that do not require HPLC access and another variation may be used for Example F-18 Product 1A and similar products that require an HPLC step. Module design approach for FDG and similar cassettes may also include consideration to the needs of the module that would support other products. To provide maximum flexibility, the Multi-Synth unit may accommodate six modules contemporaneously. For a given processing run, these six modules may all be the same type, such as FDG synthesis modules, or they may include a mixture of several types of synthesis modules, such as FDG and Example F-18 Product 1A modules, and one or two HPLC modules.

**[0193]** Synthesis modules in accordance with aspects presented herein may include features to: locate and support the cassette/reagent pack; provide connections between the cassette and the rest of the system for fluids and gases such as water, inert gas and vacuum lines, as well as disposable connections for the input line from the splitter, the output product line, and the waste line; provide one or more fluid pumps, and a multiple number of pneumatic valves and actuation lines; provide sensor and electrical connections for heaters, temperature sensors, pressure sensors, etc.; provide location and support for multiple radiation sensors; engage the reagent pack to the cassette and the cassette to the module when commanded, and to hold the cassette and reagent pack firmly to each other and to the module until synthesis is completed; eject the cassette/reagent pack from the module upon command; and do all of the above with minimum input required from the operator and so as to reduce and/or minimize user errors.

**[0194]** FIGS. **39-40** present an overview of one example synthesis module design approach, in accordance with aspects presented herein.

**[0195]** In one example variation, reliable connections between the cassette and the module and between the module



and the Multi-Synth unit that require little or no input from the operator are provided. The connections between the cassette and the module in this variation may be made automatically for each cassette processed. The connections between the module and the Multi-Synth may be made automatically, for example, any time a module is installed. In addition, the fluid lines that supply the cassette with fluid from the splitter, transfer the final product from the cassette to the hot cell, and connect the cassette to the waste vessel may all be made accessible for frequent replacement. Based on these features, because of the limited space available with six modules in one mini-cell, as well as to limit the need to pull the entire Multi-Synth unit forward in the mini-cell to reach connections on the back side of the module, the following features may be included. The cassette to module connections may be implemented via a feature or features to automatically pull the cassette firmly against the module front plate just prior to initiation of synthesis; connections may be provided that are made automatically as the cassette is pulled against the module. Module to Multi-Synth connections may be achieved by implementing features that automatically make the fluid, gas, and electrical connections as the module is manually moved into position in the Multi-Synth. Additionally, connections of the replaceable line sets may be made by pulling a module partially forward in the Multi-Synth to provide access to the connectors.

**[0196]** The module design approach may incorporate a front mounting plate that interfaces with the cassette. This plate may incorporate multiple fittings (e.g., 4 for the FDG compatible module) to connect to tubing from pneumatic valves. Pneumatic passages from the mounting plate to the cassette may be sealed, such as by gasket material. The front mounting plate may also incorporate custom luer fittings, for example, for connection of fluid lines to the cassette. These fittings may use self-aligning, spring loaded components in the module, for example, in order to accommodate alignment of multiple fittings and to provide a uniform and controlled press fit for each fitting to prevent leaks. In order to avoid fluid lines that transfer radioactive fluids to and from the cassette being routed through the module, four of these luer fittings may be located on a separate side section of the module front plate assembly. This side section may extend beyond the side wall of the module and permit connections of the disposable fluid lines to the back side of this section, where they are assessable and do not pass through the module itself.

**[0197]** The module to Multi-Synth backplane connections may include fluid connections, inert gas connections, vacuum connections, electrical power connections, sensor connections, and computer and controller interface connections, for example. To avoid having to pull the entire Multi-Synth unit forward in the mini-cell to gain access to the connections at the back of the module, in some variation, connections may be made simply by sliding a module into the Multi-Synth unit. These connections may be robust, leak proof, and self aligning. In order to achieve adequate alignment for the couplings and connectors, some variations may include tapered guide pins that provide alignment as the module approaches the connectors. A locking pin or similar device may be engaged to hold the module in place once the connections are made, to, among other things, prevent unintentional disengagement of the connectors.

**[0198]** For FDG and similar products, for example, the module may contain one positive displacement pump. This pump may be used to provide metered volumes of water to the

cassette. Since this pump is only used to provide cassette flushing after the synthesis is complete, flow rates and accuracy requirements may not mandate the use of a precision pump. The determination of activity levels in the incoming fluid from the cyclotron and splitter may be based on radiation sensing in the splitter unit. The determination of final product activity levels may be made in the hot cell. The use of radiation sensors in the synthesis units may primarily be for diagnostic purposes. In one example approach, for use, for example, with the synthesis of FDG and similar products, three radiation sensors may be provided. These sensors may be located in the module and positioned to provide diagnostic level data at three locations in the cassette: 1) within the QMA cartridge; 2) in the reaction vessel; and 3) within the first tC-18 or similar cartridge. These radiation sensors may be similar in design to the sensors used in the splitter, but may incorporate less tungsten shielding and a different geometry, for example, due to the space constraints in the module and cassette and the less demanding accuracy and range requirements in this application.

**[0199]** The modules may include features to enable pulling of the cassette and reagent pack together, and to hold them tightly against the module front plate in order to implement the fittings and sealing functions during the synthesis process. In one variation, one or more mechanical actuators are provided to pull the disposable reagent pack tightly against the module and hold them during synthesis. In the example configuration shown in FIGS. 39-40, two pneumatic actuators provide the motion and clamping force. When the actuators are fully extended, the linkage device opens the clamping devices to permit the operator to place the cassette and reagent packs on the module guide pins. Just prior to synthesis, the pneumatic cylinders may be commanded to pull the disposables into operating position. As the cylinders move the clamping devices inward within the housing, as shown in FIGS. 39-40, the biased (e.g., spring loaded) linkage may close the clamps over the disposables, and in the fully inward position, the spring system may control and limit the clamping pressure. After completion of the synthesis process, and upon command from control system, the pneumatic actuators may extend and eject the disposable reagent pack. Depending on the control system inputs, the actuators may move far enough to force the disposable reagent pack off the module guide pins, so that it is able to be dropped into a chute or slot, for example, or the extension may be limited so that the connectors and seals are disengaged, but the disposable reagent pack remains on the guide pins for later removal.

#### Synthesis Cassette

**[0200]** Aspects may include a chamber provided in a fluid handling cassette, arranged to allow the controlled movement of fluid through the remote action of pneumatic valves. The chamber may be a reaction vessel that having a substantially three-dimensional configuration, with an elongated shape and a relatively thin third dimension. For example, the reaction vessel may be flat, kite-shaped and oriented vertically, which allows liquid and vapor to separate and create a liquid level inside the vessel. Also, the thin third dimension of the vessel may be thin enough to force the liquid to spread over a predominantly flat wall through which heat or cold may be transmitted. The sides of the vessel may be tapered near the bottom in order to enhance the mixing effect of gas entering from the bottom port, and the sides may be tapered to provide



a full evacuation of the liquid through the bottom port when the reaction process is complete.

**[0201]** In some variations, the synthesis process is performed in a small device that conducts the processing with smaller quantities of fluids. Since the maximum activity level goals are significantly higher than currently processed in related art MX units, this approach means that the activity concentrations may be much higher. For example, if the batch size is 30 Ci and the typical fluid volumes used are 25 percent of current volumes, the activity concentration may be about 8 to 16 times higher than encountered in 5 to 10 Ci batches for units of the related art. In some variations, sufficient additional room is provided in the cassette so that the volumes for individual process steps can be increased or decreased based on the needs of hardware or other constraints.

**[0202]** In addition to selecting cavity and fluid volumes, other variable features for the synthesis cassette may include fluidics, heating and cooling, reaction vessel configuration, sensor access, connections and sealing, and materials selection.

**[0203]** One example approach for electrical connections to the cassette is to use biased (e.g., spring-loaded) or other suitably engageable contacts, such as pogo pins or battery springs, to make connections when the cassette is clamped against the module. Where possible, the need for electrical components in the disposable cassette is avoided. An embedded temperature sensor in the cassette, near the reaction vessel, may be needed for some implementations to control heating processes, for example. Elsewhere in the cassette, activity may be monitored using non-contacting radiation sensors located in the module and aimed at SPE columns, where the reagents involved in the synthesis process may stand the greatest risk of being lost, for example.

**[0204]** FIG. 41 shows an exploded view of various portions of an example synthesis cassette, in accordance with aspects presented herein. FIG. 41 illustrates a cassette main layer 4102, a cover-plate layer 4104, and a membrane layer 4106.

**[0205]** Certain features of the cassette for some implementations may vary from those depicted in FIG. 41. One such feature that may vary is the cassette main layer 4102, which may be formed from two different materials, such as a highly thermally conductive material around portions of the reaction vessel cavity, and a low thermal conductivity material elsewhere. Another varying example may be the cover plate 4104 assembly with piercing posts, which may integrate the piercing posts as features of an injection molded part containing locally raised contact surfaces for the reagent pack assembly and that may allow large clamping forces to be transmitted, while limiting the compression of the o-ring seals around each piercing feature.

#### Reagent Pack

**[0206]** In accordance with aspects presented herein, the reagent pack is or comprises the disposable component that contains the processing fluids and powders that are needed to synthesis a specific radiopharmaceutical product. Since each radiopharmaceutical product requires a unique combination of reagents, both by type and by volume, each product requires a unique reagent pack. These reagent packs may need to be stored under conditions appropriate for the reagents, and then assembled with the synthesis cassettes at the time the mini-cell is loaded for the next processing runs. Reagent packs may have unique mechanical features to pre-

vent improper orientation on the cassette and to make sure that the cassette and reagent pack are compatible.

**[0207]** In some variations of the reagent pack, several of the more commonly used fluids, such as acetonitrile, ethanol, and water are supplied from bulk supply lines through the module. This approach reduces the size and complexity of the reagent pack. In other variations, the reagent pack stores all of the fluids and powders that are to be used in the cassette, except the final flushing water, such as may be used after the product has been sent to the hot cell.

**[0208]** For many radiopharmaceutical products, one or more of the reagents may need to be stored in powdered form and then mixed just prior to introduction into the cassette. The cassette and/or the module may need to provide pumping and valving provisions to accommodate this mixing process. For some products, one or more of the reagents may need to be stored under conditions that are not appropriate for the remainder of the reagent pack, such as at temperatures below freezing. For these products, the reagent pack may need to accommodate one or more small reagent capsules, for example, which are inserted into the reagent pack just prior to installation in the mini-cell.

**[0209]** FIGS. 42 and 43 illustrate exploded views of various features of an example reagent pack, in accordance with aspects presented herein. FIG. 42 illustrates an outer cover plate 4202, a gasket layer 4206, a reagent pack main layer, and a cassette facing foil layer, each having an opening configured to receive a reagent container 4204. FIG. 43 illustrates an additional view of these layers.

**[0210]** In some variations, the reagents may be stored in individual cavities in the Reagent Pack main layer. The cavities in these variations are completed by the permanent assembly of an outer cover plate to the main layer. Each reagent cavity may have two exits on the cassette-facing side, a fluid exit and a vent. After the cavities are filled with reagent, both exits are sealed by a foil layer. When the reagent pack is assembled by the user onto the module and in front of the cassette, standoffs prevent the foil from being immediately pierced by the cassette assembly. When the system is ready to begin synthesis, for example, the standoffs may be removed, or overcome, by the clamping mechanism. The clamping force thereby causes the cassette assembly to pierce the foil of the reagent pack assembly, merging the fluidic circuits of the two disposable parts with the durable fluidics of the module. In one example implementation, one or more O-rings or other sealing mechanisms are incorporated around each piercing feature to seal the merged fluidic system against external leakage.

**[0211]** Materials may be selected to allow extended storage of reagent pack assemblies before use. Particularly difficult solvents may require additional protective layers in the form of inserts, or coatings, for example. Different materials may also be selected for the main layer of the reagent pack, according to the process for which the pack is intended.

**[0212]** Examples of volumes and types of fluids and powders that may be stored in reagent packs, in accordance with aspects presented herein, are included in the tables of FIGS. 9 and 11.

**[0213]** As shown, for example, in FIG. 41, the orientation angled piercing posts may be important in some implementations to control, for example, where the flap of foil ends up (see, e.g., Photostat in FIG. 44 of example bent foil flaps 4402 produced using angled piercing posts, in accordance with aspects presented herein). In some directions, the flap of foil



could partially obstruct the flow of reagent if a proper angle is not produced. For example, folding the flap directly away from the flow direction may create a region of trapped fluid.

**[0214]** The size and shape of the piercing post for use in foil pierced mixing of components requires a good match of foil thickness and reagent cavity opening clearance. The O-rings may be sealed acceptably, for example, but the design must also limit their compression by including other contacting features between the reagent pack and the piercing plate. Shorter posts may be used so long as they retain enough engagement to fold the foil flap out of the way.

**[0215]** By re-routing a solvent back into the reagent pack, a powdered reagent may be mixed by the flow of solvent through the cavity storing the dry powder. The dry cavity may be designed to store the powder near where the solvent enters, and include a serpentine path before leaving the reagent pack to ensure complete mixing.

#### HPLC Cassette

**[0216]** In one example implementation of a system in accordance with aspects presented herein, several radiopharmaceutical formulations that are of interest, such as Example F-18 Product 1A, may require synthesis steps that include processing in an HPLC unit for purification. The size and complexity of the components used in commercial HPLC units make it impractical to incorporate the HPLC functionality in the synthesis cassettes and modules. In some variations, therefore HPLC functionality is incorporated in separate modules dedicated to that purpose, e.g., the HPLC units **3404** illustrated in FIG. **35**. Since the system may be intended to incorporate up to six modules in a mini-cell, for example, one or more of the six synthesis modules may be replaced by HPLC modules when formulations such as Example F-18 Product 1A are to be processed. In this configuration, an HPLC module may be installed next to an Example F-18 Product 1A synthesis module with appropriate fluid connections between the modules. Even with this module approach, size constraints may require that some of the HPLC components be located outside the mini-cells.

**[0217]** Components in example HPLC units may include an injection loop **4502**, to gather and then inject the sample into the HPLC flow path; an HPLC column **4504** that contains the appropriate packing material for the application; a high pressure pump **4506** to deliver a mobile phase (solvent) and the sample through the tightly packed column; a source **4508** for the appropriate mobile phase solvent; one or more detectors **4510**, to determine when the selected fluid constituent is exiting the column; a selector valve **4512** to route the fluid exiting the column either to waste or back to the synthesis cassette; and control components and sensor instrumentation.

**[0218]** Implementations of the system may provide a platform to synthesize a variety of radiopharmaceutical formulations requiring HPLC processing. Several approaches to reduce the component and/or module swapping may be used to accommodate a variety of formulations, including the following: revising or adapting the radiopharmaceutical formulations to use a smaller number of different column packing materials and solvents; this approach may reduce the number of HPLC options to perhaps two or three, but may require changes in the formulation recipes, which could in turn lead to licensing and/or FDA approval complications; varying HPLC modules for each formulation, and ensuring that these modules relatively easy to swap out; different solvent sources may also be needed; varying the HPLC module to make it

relatively easy to swap out of the column, so that the appropriate column is in place for the next formulation that is scheduled; different solvent supplies may also have to be available for this approach; and using an HPLC module that incorporates a column selector device and provides multiple columns to choose from without need for hardware swapping; this approach may also require a pumping system that can select from multiple solvent sources without component swapping.

**[0219]** In multiple column selector variations, the HPLC module may incorporate a four-way selector valve and four HPLC columns, for example. FIG. **46** illustrates an HPLC module having four HPLC columns **4504**. Each of these columns may contain a different packing material if desired, or several columns may contain the same type of material, with one being used as a backup for the other. The injection loop may be placed in the circuit ahead of the four-way selector. Since different formulations may require different solvents, a mobile phase pump that is able to select among four different solvent sources may be used. This pump may also have provisions to flush line sets in between applications.

**[0220]** A schematic of an example HPLC system in accordance with aspects presented herein is shown in FIG. **45**. The HPLC module shown in FIG. **45** includes two detectors, a radiation sensor **4514** and an ultraviolet (UV) sensor **4510**. The outlet fluid from the columns passes by the UV sensor and then the radiation sensor. The UV sensor alerts the system that the constituents of interest are exiting the column, and the radiation sensor determines when the selected radioactive material is exiting the column. This data may be used to direct the selector valve, in order to send the desired material to the return line to the synthesis cassette, for example, rather than the waste line.

**[0221]** Due to space constraints and the radiation activity levels inside the mini-cell for some variations, as many of the HPLC components as practical may be located externally to the mini-cell. Such external components may include, for example, the solvent pump and solvent supply systems, the sensor electronics, and the control system for the selector valves.

**[0222]** The connections to the synthesis cassettes may be made by connectors at the side of the module nearest the synthesis modules. As the synthesis cassette is pulled into contact with the synthesis module, for example, the cassette may then also make connections to the HPLC module.

**[0223]** The columns shown in the example implementation shown in FIG. **45** are full-size 250 mm long columns as may be used, for example, in Example F-18 Product 1A processing. It may be possible to reduce the length and/or diameter of the columns for some formulations, based on reduced fluid volumes that are expected to be used in some variations of synthesis processes in accordance with aspects presented herein. Shorter or smaller diameter columns may be used with the same selector valve by making minor connection line changes, for example.

**[0224]** An overview of one example design approach to the HPLC module in accordance with aspects presented herein as outlined above is illustrated in FIGS. **46** and **47**. Example commercial components that may be used for certain features include: a Solvent Pump, such as a Dionex Quaternary Analytical Pump (LPG 3400SD); a four-way Column Selector, such as a VICI Cheminert HPLC Column Selector unit (C5-



2004EMHD); and an injection Valve and Loop, such as a RHEODYNE, RV700-114, 2-POS, 6-PORT Motorized valve.

**[0225]** Additional details of such an HPLC may be found in Provisional Application No. 61/508,349, titled “System for Radiopharmaceutical Preparation Involving Solid and Liquid Phase Interactions,” filed on Jul. 15, 2011, the entire contents of which are hereby incorporated by reference herein.

#### Disposable Columns

**[0226]** Various components of the HPLC module may be replaced periodically, or be changed when used for synthesizing different radiopharmaceutical compounds. Typically, a component of the system may be replaced while the system is not operating to prepare a radiopharmaceutical. For example, after a column **3404** is used in multiple runs of the HPLC module to purify radiopharmaceutical products, it may deteriorate or not function effectively to separate the desired radiopharmaceutical material. Failure of a column is usually detected, for example, by a large pressure increase in the pump at a set mobile phase flow rate or a longer process time for separating the desired radiopharmaceutical material than is typically required. Such a failure may occur after about 10 to 100 runs of the HPLC module with that column.

**[0227]** In accordance with aspects presented herein, the deteriorated column may be replaced with a different column. In addition, a column having a specific stationary phase may be required to produce a particular radiopharmaceutical compound. Thus, according to aspects presented herein, a column in an HPLC module having one stationary phase may be removed from the HPLC module and replaced with another column that has a different stationary phase, for example. To simplify the removal of a column from the HPLC module, at least one edge of the container that houses the HPLC module’s components may be removed and columns may be positioned at an edge of the HPLC module.

#### Automated Quality Control (QC) Platform/Lab Information Management (LIM)

**[0228]** In accordance with aspects presented herein, an automated QC system and apparatus may be used, for example, for radio-synthesized tracers, covering a plurality of tests, which assess, for example, particle and color content (clarity), filter membrane integrity, pH value, residual solvent volume, Kryptofix concentration, bacterial endotoxins concentration, radionuclidic identify, radionuclidic purity, radiochemical identity, radiochemical purity, and sterility test.

**[0229]** The automated QC system and apparatus may advantageously record documentation and archive the materials used in the QC process and report various testing results in compliance with the current Good Manufacturing Practice (cGMP) regulations, as well as title 21 CFR Part 11 of the Code of Federal Regulations regarding the Food and Drug Administration (FDA) guidelines on electronic records and electronic signatures in the United States. Aspects also enable self-calibration of all of the tests with reporting capabilities in real time. In one aspect, simplified and fully automated QC operation is enabled by facilitating each of the above tests in an efficient manner (e.g., in less than 30 minutes). The test results may be quantitative, and multiple tests may be advantageously performed in parallel. As a result, the test results

may be more reliable, and the whole process may be more economical and efficient, as time and labor for the QC are significantly reduced.

**[0230]** Additional details regarding the Quality Control aspects may be found in U.S. Provisional Application No. 61/508,353 titled “Method and System for Automated Quality Control Platform,” filed on Jul. 15, 2011, the entire contents of which are hereby incorporate by reference herein.

#### Sterile Vial Fill Subsystem and Methods

**[0231]** To create an aseptic environment for the production of pharmaceuticals, a special clean air “canopy” or laminar flow hood, for example, is often used, wherein high-efficiency particulate air (HEPA) filters are provided in conjunction with a closed containment structure, within which the pharmaceuticals can be prepared. The interior environment of the containment structure is closely monitored, for example, by a particle counter, to determine the airborne particulate density of possible contaminants. However, when preparation of the pharmaceutical includes a radioactive material, the aseptic environment described above must also be shielded. It is very difficult to combine a shielded enclosure with a filtered environment without compromising the ability to produce a radiopharmaceutical compound efficiently.

**[0232]** Furthermore, present procedures for dispensing radiopharmaceuticals into final product vials for delivery to one or more patients often involves accessing and extracting the radionuclide product for an individual procedure from a bulk product vial. The bulk product vial, which is contained in a shielded enclosure to minimize exposure of the technician to radiation, is typically accessed by one or more technicians using a syringe to puncture a resealable membrane of the bulk product vial in order to extract a quantity of the radioactive component, introducing a chance that contaminants can be introduced into the bulk product vial.

**[0233]** To decrease the chance of contamination by multiple punctures of a syringe, it has been proposed to use an automated syringe that automatically draws material from the bulk product vial into each of the individual vials. However, even if a syringe pump, for example, reduces the chance of contamination by reducing the number of times the bulk product vial membrane is punctured, each plunge of the syringe after the initial plunge risks contamination through airborne particles, for example, being drawn in through the back of the syringe. Additionally, syringes can limit the size of a dose being dispensed.

**[0234]** Accordingly, there is a need for improved vial filling systems that may promote a more efficient setup and procedure for dispensing radiopharmaceuticals in a safe and effective manner that guarantees the integrity of the radiopharmaceutical every time.

**[0235]** In accordance with aspects presented herein, an example sterile vial fill subsystem is a closed path system that incorporates features and methods to provide for aseptically dispensing finished radiopharmaceuticals into receiving vessels, such as a Quality Control vial, a sterility vial, and/or final product vials. The system is designed with disposable components that provide users safe and efficient mechanisms for aseptic assembly of the system, as well as removal and disposal of those components that are exposed to radioactivity during use of the system. Moreover, by automating the dispensing process in a closed system, the chance of contamination associated with current systems and methods, includ-



ing, for example, automated syringes, may be substantially reduced or eliminated altogether.

[0236] The closed path vial system may include a bulk product vial for receiving a bulk quantity of a radiopharmaceutical product, a peristaltic pump operated by a stepper motor for precise control and delivery of the product from the bulk product vial to the receiving vessels, a dispensing manifold assembly to which may be coupled multiple receiving vessels for receiving the product, as determined by an automated control system, an optional quality check station, and an optional waste collection system. Furthermore, a CAV Sensor may be incorporated into the system for receiving the radiopharmaceutical product directly from a synthesizing unit and measuring critical product properties prior to dispensing the product via the automated sterile vial fill subsystem.

[0237] As shown in FIG. 48, an exemplary closed path vial fill system 4800 may include a bulk product vial 4801, a peristaltic pump 4805, a dispensing manifold assembly 4803 to which may be coupled at least one final product vial 4804, a sterility vial 4805, an optional quality check station 4884, and an optional waste collection system 4806. A control system may be integrated into the system 4800 to provide automatic and/or manual control over various aspects of the radiopharmaceutical dispensing process. Although described herein as having one pump 4805 or one bulk product vial 4801, for example, the system may encompass multiple pumps feeding multiple fluid pathways for dispensing multiple different products without cross contamination. The potential exposure of technicians may be further reduced, as the necessity to enter the shielded environment in order to change out disposable components of the system 4800 between batches (radiation safety hazard) may be further reduced.

[0238] As shown in FIG. 48, the peristaltic pump 4805 may be a simple mechanical pump comprising a replaceable tube element and rollers 4826, for example. The rollers 4826 are conventionally provided at intervals along a radial track and rotate about a central axis to exert localized pressure on the tube element 4810, which in turn pushes a fluid through the tube element 4810 and creates a negative pressure at an inlet of the tube element 4810 for drawing additional fluid into the tube element 4810. Control of the fluid flow may be by way of a standard motor (not shown) coupled to the peristaltic pump 4805. However, as shown in FIG. 48, by attaching a stepper motor 4856, for example, to the peristaltic pump 4805, aspects of the present invention permit a much more refined degree of control over the fluid flow parameters through the tube element 4810. For example, by calibrating the rotation of the pump 4805 in accordance with the rotation of the stepper motor 4856, as determined by a number of pulses applied by the stepper motor 4856 over a given period of time, a control algorithm may be determined to accurately predict and control the amount of fluid being pushed through the tube element 4810 as a function of the number of pulses of the stepper motor 4856.

[0239] In accordance with another aspect of the invention, the control system may be used to store calibration data for each position of a final product vial 4804 along the dispensing manifold assembly 4803, permitting very precise control of the fluid flow parameters into each final product vial 4804 without the need for individual flow meters for each final product vial 4804. Although referred to herein as a final product vial 4804, the final product vial 4804 may be any

suitable vessel for receiving a quantity of the radiopharmaceutical product, including a sterility vial, final product vial, or a quality control syringe, for example.

[0240] According to another aspect of the present invention, the stepper motor 4856 may be used to operate the peristaltic pump 4805 in reverse. As such, the closed path vial fill system 4800 may be used to draw a diluting solution, such as a sterile saline solution, from a dilution container 4866, for diluting the bulk radionuclide product in the bulk product vial 4801. The dilution container 4866 may be a flexible, sterile bag comprised of a resilient PVC material, for example. As shown in FIG. 48, the dilution container 4866 may be integrated into the system 4800, preferably between the peristaltic pump 4805 and the dispensing manifold assembly 4803, by way of a valve 4865. The valve 4865 may be a three-port solenoid valve, a diverter valve, or a stopcock valve, for example, and provides closed fluid communication between the peristaltic pump 4805 and the dispensing manifold assembly 4803 when selectively actuated to a first position, and closed fluid communication between the dilution container 4866 and the peristaltic pump 4805 when selectively actuated to a second position.

[0241] As shown in FIG. 49, a sterile kit 4805 may be provided for each new compounding run of a radiopharmaceutical that includes one or more of the bulk product vial 4801, the dilution container 4866, pre-filled with the dilution solution, the filter 4870, the manifold tubes 4813 and valves 4823, and the final product vials 4804, including the vented fill caps 4824. The kit 500 may come with certain or all of the components preassembled to allow for efficient set up of the system 4800.

[0242] The kit 4805 may be aseptically assembled inside a laminar flow hood inside a clean room prior to packaging for delivery and use. The kit components may be sterilized through a gamma radiation sterilization technique, or where the final product vials 4804 may be susceptible to damage from the gamma radiation, for example, steam sterilization techniques may be used. Accordingly, the kit components may arrive sterilized with some of the components already connected. The dilution container 4866, sterility vial 4854, final product vials 4854, and vented fill caps 4824 for each sterility vial 4854 and final product vial 4804 may require cleaning. Although the inside and/or contents of each of the components may be sterile, the outside surfaces and, in particular, the septa, or resealable membranes of the vials, may be sterilized with alcohol wipes prior to use in the kit. For example, the vented fill cap 4824 packages may be opened in the laminar flow hood, however, the packages should be soaked in hydrogen peroxide or alcohol prior to placement in the laminar flow hood. The vented fill caps 4824 in the packages are sterile and therefore do not require additional sterilization upon being released from the packages when in the laminar flow hood.

[0243] As shown in FIG. 49, once sterilized in the hood, the dilution container 4866 and vials 4804/4854 may be connected to the other sterile kit components. The dilution container 4866 may be connected by inserting a needle 4862 through the dilution container's septum. A dilution tube 4864 may be connected to a distal end of the needle 4862 and connected to the manifold tube 4813 through a valve. According to another aspect of the invention, the dilution tube 4864 may be configured to connect directly to one of the dispensing ports 4832, as shown with regard to the first port in FIG. 49. Vented fill caps 4824 may be mounted to the dispensing ports



**4832** directly, or by way of the connector tubes **4834**, for example, according to the number of final product vials **4804** desired and/or to accommodate the sterility vial **4854**. The final product vials **4804** and the sterility vial **4854** may then be connected to the corresponding vial caps **4824**, as appropriate. In this manner, it may be preferable to connect the sterility vial **4854** to the dispensing port **4832** sequentially farthest from the pump **4805** as compared to the final product vials **4804**. In addition, if a mixture of vial sizes is being used in the system **4800**, larger final product vials **4804** may be arranged to connect to dispensing ports **4832** along with the smaller final product vials **4804** in any desired sequence with respect to the pump **4805**.

[0244] FIG. 50 is a schematic to further illustrate a closed vial fill system **5000** incorporating a CAV sensor **5070**. The radiopharmaceutical product **5001** may be delivered from the synthesizing unit directly to the CAV container. The CAV sensor **5070** records the concentration, activity, and/or volume components of the radiopharmaceutical product **5001**. Once the desired parameters have been measured by the CAV sensor **5070**, the peristaltic pump **5021** may be used to draw the entire volume of the radiopharmaceutical product **5001** from the CAV container **5070** for deposit into the bulk product vial **5001**. As described above in detail, the peristaltic pump **5020** may then be used to draw a dilution solution from the dilution container **5026** to dilute the radiopharmaceutical product **5001** to desired levels of concentration and activity in accordance with the measurements recorded by the CAV sensor **5070**. The diluted product may then be used to fill the final product vials **5040**, **5045**, the sterility vial **5050**, and/or the quality check syringes, for example, as pre-programmed in the control system.

[0245] Additional details of the vial filler may be found in U.S. Provisional Application No. 61/508,409 entitled "Closed Vial Fill System for Aseptic Dispensing," filed on Jul. 15, 2011, U.S. application Ser. No. 13/339,226, titled "Closed Vial Fill System for Aseptic Dispensing," filed on Dec. 28, 2011, and PCT Application No. PCT/US2011/067650, titled "Closed Vial Fill System for Aseptic Dispensing," filed on Dec. 28, 2011, the entire contents of each of which are hereby incorporated by reference herein.

#### Safety Features

[0246] Safety features may comprise any of automated Interlocks and Emergency Shutdown, operator alarms, fail safe operation, user privileges, and set point limits.

[0247] Automated interlocks may be used to initiate and perform automatic emergency shutdowns when safe operating parameters are exceeded. They may be also used to prevent processes or equipment from being started out of sequence with respect to other equipment in a manner that would present a safety hazard or to prevent designated processes or equipment from being started if other equipment, critical to the safety of the process, is nonfunctional.

[0248] Operator alarm conditions may comprise events or parameters that are predetermined to require operator attention or response. Examples of alarm conditions are a process variable being out of the desired or safe operating range, equipment such as a pump or other device failing to run when commanded, or an alarm signal from an outside source, such as a facility fire alarm or an alarm signal from an independent controller. Alarms must be date and time stamped and logged. Alarm logs are a trouble shooting and diagnostic tool that record the sequence of alarm events and can be used to help

determine the root cause(s) of the alarm condition. Alarms may be categorized for severity and presented to the operator in a different manner according to the severity of the condition.

[0249] Fail Safe Operation of process control equipment may comprise self diagnostics and the ability of the control system to respond to faults by going into predefined fault states is an important safety feature.

[0250] User privilege levels are used to restrict access to process control operations to approved users, which helps to insure that only qualified and authorized users have access to functions that can compromise the safety of the system. User privilege levels are typically set by the system administrator and controlled through a user log-on function. For example, user levels such as Guest, Operator, Supervisor, and Administrator may be used with increasing levels of access for each level.

[0251] Set point limits may be used to limit the allowable range of set points that may be entered by an operator to values that will not compromise the safe operation of the system.

[0252] The control system architecture should also have the flexibility to accommodate any expected performance requirements. A general consideration for any process control system is that the system provides robust, reliable, and predictable operation. Industry standards for similar applications and the choice between using commercial off-the-shelf (COTS) hardware or custom hardware are considered. The physical size, location, electromagnetic compatibility, radiation shielding, and other special requirements must be compatible with the restraints of the process and installation. The system architecture should have the ability to accommodate the development process by providing control and support for development and testing of subsystems up to full system prototypes as well as the final production system.

[0253] The control system must have the ability for high speed timing and control in the order of several milliseconds. Critical communication paths must be deterministic and repeatable to provide real-time control for time-critical I/O and messaging data. This may be provided in part by the systems described herein and the system illustrated in FIGS. 50 and 51.

[0254] Data acquisition and logging, data export capability, and graphical trending of both historical and real-time data may be provided. Secure data logging may be required for regulatory purposes, therefore methods of data acquisition and storage must be compliant with pharmaceutical manufacturing requirements.

#### Control Software and Subsystem(s)

[0255] Aspects are directed to systems, methods, and devices for providing software and hardware controls for overall and various sub-portion operation that include suitable radiation and other damage and contaminant resistant features, and that allow for optional remote data collection, communication, and/or control for producing radiopharmaceuticals. Aspects of the process for producing pharmaceuticals include: 1) generating radionuclides for use in production of radiopharmaceuticals, such as via use of a cyclotron; 2) synthesizing the radionuclides generated and removing any unwanted products included with the generated radionuclides (e.g., drying and/or deprotecting the generated radionuclides); 3) measuring the quantity and activity level of the synthesized radionuclides; 4) distributively delivering the



radionuclides in appropriate quantities to a plurality of modular cassette synthesis units in a modular cassette subsystem for contemporaneous/parallel production of radiopharmaceutical output and that allow reuse and/or quick, safe, and disposable replacement of portions of the subsystem; 5) delivering appropriate quantities of non-radionuclide components to the plurality of modular cassette synthesis units as part of the contemporaneous/parallel production of radiopharmaceutical output; 6) upon production of the radiopharmaceutical output from the plurality of modular cassette synthesis units, measuring the quantity and activity level of each stream of radiopharmaceutical output; 7) purifying the radiopharmaceutical output; 8) distributively dispensing individual doses in one or more sterile vials; 9) optionally automatically producing labeling and dose related information for use with the doses; and 10) performing automated quality control on one or more extracted samples from the produced radiopharmaceutical output.

[0256] Individual systems typically used during production of radiopharmaceuticals operate on various independent software systems without interacting with other software systems involved in the production of radiopharmaceuticals. Thus, there is a need in the art for methods and systems for coordinating the production of radiopharmaceuticals to ensure that a radiopharmaceutical is produced efficiently and delivered to a patient before the radiopharmaceutical decays. Moreover, there is a need in the art for automating the production process of radiopharmaceuticals in order to reduce the time required for production, the amount of training required for operators of the production system, the amount of operator error and/or the number of failed batches during the production process, in addition to producing a high-quality product and performing efficient quality control contemporaneously with or subsequently to the production of radiopharmaceuticals.

[0257] FIG. 51 illustrates a system similar to FIG. 1. Cooperation between system components in FIG. 51 allows increased production by providing increased efficiency of feed and accuracy of both characteristics and volume of radionuclide raw material input to the production process. It should be appreciated that any of the systems 5106-5126, may comprise wired, wireless, and/or fiber optically communicating devices and/or other computing devices. Wireless devices, for example, may include any suitable mobile, portable computing or communications device, such as a cellular device, that may connect to an access network 5104. For example, wireless devices may include a cellular telephone, a navigation system, a global positioning system (GPS), a computing device, a camera, a personal digital assistant (PDA), or other handheld device having wireless connection capability, among other devices. It should also be appreciated that control platform 5102 may comprise a server and/or computing devices that may include, for example, any suitable mobile or fixed computing device connected to a network.

[0258] Control platform 5102 may use the input received from one or more systems, such as cyclotron system 5106, splitter system 5108, synthesis units system 5110, purifying output system 5112, output measurement system 5114, vial filler system 5116, pharmacy dispensing and distribution system 5118, quality control system 5120, labeling system 5122, billing system 5124, and/or logistic system 5126 to create an environment for controlling and/or managing the production and distribution of radiopharmaceuticals.

[0259] In an aspect, control platform 5102 may be used to communicate between the one or more systems 5106-5126.

For example, control platform 5102 may notify the various systems 5106-5126 when a particular system should be used in the process of manufacturing and/or delivering radiopharmaceuticals. Thus, control platform 5102 may be used to coordinate the sequence and timing of production of radiopharmaceuticals. For example, control platform 5102 may receive input from cyclotron system 5106 indicating that the cyclotron system 5106 is finished producing radioactive output, such as, but not limited to, Fluorine 18, C11, NH3. The received input from cyclotron system 5106 may include, but is not limited to, the following information relating to the production of the radioactive output: an amount of output produced; a start time for the production; an end time for the production; a total production time (e.g., a total amount of time cyclotron system 5106 spent producing the output); an order receipt time; and/or a location of the cyclotron system 5106 (e.g., the location of the lab where the cyclotron system 5106 is housed), among other information relating to the production of radioactive output.

[0260] Control platform 5102 may process the received information from cyclotron system 106 and notify splitter system 5108 that the radionuclide, e.g., F-18 is ready to be delivered into the splitter. In addition, control platform 5102 may be used to distribute the radioactive output produced by cyclotron system 5106 to splitter system 5108 for use in the next step of processing the radiopharmaceuticals. It should be appreciated that similar information, as discussed above, may be received from the one or more systems 5106-5126. It should be appreciated that control platform 5102 may be involved in each stage of the production and/or distribution process of radiopharmaceuticals, and may be used to coordinate the sequence of production of the radiopharmaceuticals. Control platform 5102 may be able to track the progress of the radiopharmaceutical product, as the product moves through the various systems 5106-5126 and use the information received from the one or more systems 5106-5126 to notify the various systems 106-126 when a particular system should be used. By communication with the various systems 5106-5126, control platform 5102 may increase the efficiency of production of radiopharmaceuticals. Control platform 5102 may also be used to communicate with a remote monitoring station which may be able to further support production of radiopharmaceuticals (e.g., mission control) and/or maintenance of the production system.

[0261] In an aspect, control platform 5102 may be used to increase the number of simultaneous product synthesis being performed by synthesis unit 5110 in multiple modules of a multisynthesis unit based upon, for example, need, volume and/or activity. For example, control platform 5102 may direct synthesis unit 5110 to perform parallel synthesis of one or more different radiopharmaceuticals simultaneously. Control platform 5102 may be used for example, to direct the amount of radioactive output, such as F-18, C11 or NH3 produced by cyclotron 5106 and distribute via the splitter 5108 the radioactive output based upon the amount of activity needed to produce the one or more products. For example, control platform 5102 may direct the correct amount of F-18, C11 or NH3 from splitter 5108 to one or more synthesis units 5110 to perform the requested synthesis.

[0262] It should be appreciated that a number of syntheses may be capable of occurring at the same time and being controlled by control platform 5102. In an aspect, up to 12 syntheses may be performed by synthesis unit 5110 in 2 multisynthesis units. In another aspect, control platform 5102



may control more than one synthesis unit **5110**, with each synthesis unit **5110** running parallel synthesis to produce one or more different radiopharmaceuticals.

[0263] In an aspect, control platform **5102** may interface with vial filler **5116** to ensure that the produced radiopharmaceuticals are filled in the correct quantities amongst several bulk product vials to be distributed to pharmacies. For example, control platform **5102** may ensure that a correct quantity of a radiopharmaceutical is distributed to the correct pharmacy at the correct time.

[0264] In addition, control platform **5102** may monitor and/or control the quantity of bulk product to pharmacies by receiving and/or providing information to vial filler **5116**. In an aspect, control platform **5102** may communicate with the pharmacy **5118** and monitor the individual patient dose drawn at the pharmacy. For example, the shielding of the device delivering the radiopharmaceutical to the patient may have a sensor embedded in the housing that may provide patient dosage information to the pharmacy dispensing distribution system **5118**. Patient dosage information may include, but is not limited to, the amount of radiopharmaceutical being injected into the patient, the remaining radiopharmaceutical in the housing after providing the dosage to the patient, and the weight of the housing after providing the dosage to the patient, among other patient dosage information. Control system **5102** may receive the patient dosage information provided by pharmacy dispensing distribution system **5118** and compare the received patient dosage information with the amount of radiopharmaceutical originally delivered to the patient and determine the amount of radiopharmaceutical remaining in the housing after providing the patient dosage. Control system **5102** may use the patient dosage information to determine whether a proper amount of radiopharmaceutical was delivered to the patient.

[0265] In addition, control platform **5102** may use the input received from one or more systems **5106-5126** to track radiopharmaceuticals from the production stage to the patient dosage. In an aspect, a batch record number may be linked to the one or more radiopharmaceuticals produced via system **5100** and stored in a data store on control platform **5102**. For example, the batch record number may be linked to and/or associated with a specific dose for a particular patient from a batch of radiopharmaceutical produced. Thus, control platform **5102** may be able to use the batch record number associated with the specific dose provided to the patient to trace the radiopharmaceutical to the original source of the radiopharmaceutical, e.g., the materials used for production and/or the location where the radiopharmaceutical was produced. In an aspect, the batch record number may be included on a hardware device delivering the radiopharmaceutical to the patient. For example, the batch record number may be a chip, such as radio-frequency identification (RFID) chip, embedded on the hardware device. In addition, the batch record number may be printed on the shield of the device delivering the radiopharmaceutical to the patient.

[0266] In one variation, the input received from the one or more systems **5106-5126** during the production and/or delivery of radiopharmaceuticals may be used by control platform **5102** to trace the location and/or source of the materials used during production of radiopharmaceuticals. For example, if a patient receives a radiopharmaceutical and experiences an adverse reaction to it, the control platform **5102** may be used to aid a pharmacy in determining whether an error occurred during the production of the radiopharmaceutical. Control

platform **5102** may receive input regarding the particular radiopharmaceutical supplied to the patient, e.g., a batch record number of the radiopharmaceutical, and may use the input received from the one or more systems **5106-5126** during the production of the radiopharmaceutical to determine, for example, production factors relating to the radiopharmaceutical supplied to the patient. Production factors may include, but are not limited to, a location where the particular radiopharmaceutical was produced, materials used during the production process, a time when the radiopharmaceutical was produced, and/or an amount of time the radiopharmaceutical spent in transit, among other production factors. It should be appreciated that the control platform **5102** may generate the production factors in real-time or near real-time, and therefore, provide the received information for the particular radiopharmaceutical to the pharmacy, and thus, to the provider quickly to aid in determining the cause of a patient's adverse reaction to the particular radiopharmaceutical.

[0267] Control platform **5102** may further use the input received from one or more systems **5106-5126** for performing quality control measures during the production of radiopharmaceuticals. Quality control measures may include, but are not limited to, checking and/or testing the status of each of the systems **5106-5126**, checking the environment surrounding systems **5106-5126**, testing outputs produced by each of the systems **5106-5126**, and/or performing testing on samples of the radiopharmaceuticals produced by system **5100**, among other quality control measures. In an aspect, a regulatory agency, such as the Food and Drug Administration (FDA) regulates the production of radiopharmaceuticals and requires a quality threshold be met during the production. Quality control system **5120** may be used, for example, to generate one or more quality reports relating to the quality of the radiopharmaceuticals produced by system **5100**. Quality reports may include, but are not limited to: analytical tests performed on the product; total yield of the products; failure reports for the product; failure reports for the one or more systems used to manufacture the product; and/or operator error reports, among other quality reports. Quality control system **5120** may interface with each individual system when performing the quality control measures.

[0268] In an aspect, control platform **5102** may generate alerts indicating a failure in the process and/or a delay in the process. For example, alerts may be generated when one or more of the systems **5106-5126** malfunctions and/or stop working. Alerts may be used by control platform **5102** to stop the manufacturing process and/or redirect the workflow of the manufacturing process. For example, if the control platform receives an alert that a cyclotron in a lab is malfunctioning, the control platform may direct new radiopharmaceuticals orders to cyclotrons in other labs until the control platform receives an update clearing the alert. By having the capability to redirect the workflow upon receiving alerts indicating a problem during production, the control platform may be able to maximize the use of available resources and maintain production of the radiopharmaceuticals within a required time frame. Thus, the control platform may be able to get the radiopharmaceutical to the patients within a timely manner and maximize the effectiveness of the radiopharmaceutical received by the patients.

[0269] In another example, alerts may be generated if an environment surrounding the one or more systems **5106-5126** becomes unstable. For example, the environment surrounding the one or more systems **5106-5126** may be required to



remain within a temperature range to ensure the safety of the equipment and/or the individuals involved in the production process. If control platform **5102** detects that the temperature of the environment exceeds the desired temperature range, control platform **5102** may generate an alert indicating the temperature of the environment exceeded the temperature range and stop the production process and/or alter the temperature controls in the environment. In addition, control platform may be able to redirect the workflow of the production, as discussed above upon receiving the alert.

[0270] In one aspect, control platform **5102** may receive input from logistics system **5126** to ensure that the production and distribution of radiopharmaceutical may be ordered, manufactured, and distributed to a patient within a required time period (e.g., 24 hours). Logistics system **5126** may store information relating to the production capabilities factors of one or more production sites (e.g., a lab where the radiopharmaceuticals are produced). Production capabilities factors may include, but are not limited to, the amount of available materials at the production site, the workloads of the system components at the production sites, and/or available system components at the production sites, among other production capabilities factors.

[0271] Control platform **5102** may manage the workload of the systems **5106-5126** by adding and/or removing processes from the one or more systems **5106-5126** based upon, for example, available resources at a particular production facility and/or pharmacy. In an aspect, control platform **5102** may receive a request for a quantity of a particular radiopharmaceutical, and may place an order with an available cyclotron **5106** and location which has the proper materials to produce the requested radiopharmaceutical. In addition, control platform **5102** may distribute workloads for the one or more systems **5106-5126** and/or redistribute the workloads to maximize, for example, the available materials at the one or more systems **5106-5126**. For example, if splitter **5108** has enough materials for the received request, control platform **5102** may redirect which synthesis unit **5110** the materials are directed to from splitter **5108** based upon the received request. In addition, if another production site has more available resources, the control platform **5102** may move the production of the requested radiopharmaceutical to the other production site with more available resources.

[0272] Aspects presented herein may be implemented using hardware, software, or a combination thereof and may be implemented in one or more computer systems or other processing systems. In an aspect, features are directed toward one or more computer systems capable of carrying out the functionality described herein. An example of such a computer system **5200** is shown in FIG. 52.

[0273] Computer system **5200** includes one or more processors, such as processor **5204**. The processor **5204** is coupled to a communication infrastructure **5206** (e.g., a communications bus, cross-over bar, or network). Various software aspects are described in terms of this example computer system. After reading this description, it will become apparent to a person skilled in the relevant art(s) how to implement aspects hereof using other computer systems and/or architectures.

[0274] Computer system **5200** may include a display interface **5202** that forwards graphics, text, and other data from the communication infrastructure **5206** (or from a frame buffer not shown) for display on a display unit **5230**. Computer system **5200** may include a main memory **5208**, preferably

random access memory (RAM), and may also include a secondary memory **5210**. The secondary memory **5210** may include, for example, a hard disk drive **5212** and/or a removable storage drive **5214**, representing a floppy disk drive, a magnetic tape drive, an optical disk drive, etc. The removable storage drive **5214** may read from and/or write to a removable storage unit **5218** in a well-known manner. Removable storage unit **5218**, represents a floppy disk, magnetic tape, optical disk, etc., which may be read by and written to removable storage drive **5214**. As will be appreciated, the removable storage unit **5218** may include a computer usable storage medium having stored therein computer software and/or data.

[0275] Alternative aspects may include secondary memory **5210** and may include other similar devices for allowing computer programs or other instructions to be loaded into computer system **5200**. Such devices may include, for example, a removable storage unit **5222** and an interface **5220**. Examples of such may include a program cartridge and cartridge interface (such as that found in video game devices), a removable memory chip (such as an erasable programmable read only memory (EPROM), or programmable read only memory (PROM)) and associated socket, and other removable storage units **5222** and interfaces **5220**, which allow software and data to be transferred from the removable storage unit **5222** to computer system **5200**.

[0276] Computer system **5200** may also include a communications interface **5224**. Communications interface **5224** may allow software and data to be transferred among computer system **400** and external devices. Examples of communications interface **5224** may include a modem, a network interface (such as an Ethernet card), a communications port, a Personal Computer Memory Card International Association (PCMCIA) slot and card, etc. Software and data transferred via communications interface **5224** may be in the form of signals **5228**, which may be electronic, electromagnetic, optical or other signals capable of being received by communications interface **5224**. These signals **5228** may be provided to communications interface **5224** via a communications path (e.g., channel) **5226**. This path **5226** may carry signals **5228** and may be implemented using wire or cable, fiber optics, a telephone line, a cellular link, a radio frequency (RF) link and/or other communications channels. As used herein, the terms “computer program medium” and “computer usable medium” refer generally to media such as a removable storage drive **480**, a hard disk installed in hard disk drive **5212**, and/or signals **5228**. These computer program products may provide software to the computer system **5200**. Aspects are directed to such computer program products.

[0277] Computer programs (also referred to as computer control logic) may be stored in main memory **5208** and/or secondary memory **5210**. Computer programs may also be received via communications interface **5224**. Such computer programs, when executed, may enable the computer system **5200** to perform the features in accordance with aspects presented herein, as discussed herein. In particular, the computer programs, when executed, may enable the processor **5210** to perform the features in accordance with aspects of the present invention. Accordingly, such computer programs may represent controllers of the computer system **5200**.

[0278] Where aspects presented herein may be implemented using software, the software may be stored in a computer program product and loaded into computer system **5200** using removable storage drive **5214**, hard drive **5212**, or communications interface **5220**. The control logic (software),



when executed by the processor **5204**, may cause the processor **5204** to perform the functions described herein. In another aspect, the system may be implemented primarily in hardware using, for example, hardware components, such as application specific integrated circuits (ASICs). Implementation of the hardware state machine so as to perform the functions described herein will be apparent to persons skilled in the relevant art(s).

[0279] Example control system architectures may comprise, among others, any of a PLC-HMI based system, a custom hardware/custom software system, and a LabView based system. A PLC (Programmable Logic Controller), also referred to as a PAC (Programmable Automation Controller), such as Allen Bradley ControlLogix system provides process control, e.g., PLC software in ladder logic and function block programming languages may be used. A panel mounted or desktop PC may be used for the Human Machine Interface (HMI). The HMI software may use development software such as Wonderware InTouch or Rockwell RSView. A data historian such as Wonderware Historian or similar product may be used for data acquisition, data export, trending, and reporting. Custom embedded hardware may be used to interface field devices with process control provided by custom PC based and/or embedded software. The HMI and control software may be in C/C++/C# programming languages. National Instruments LabView CompactRIO hardware may be used for process control. A panel mounted or desktop PC may be used for the HMI. Both the control and HMI software may use LabView Developer Suite Core development software. The software may be written in LabView's custom graphical programming language.

[0280] In yet another variation, aspects presented herein may be implemented using a combination of both hardware and software.

[0281] FIG. 53 shows a communication system **5300** usable in accordance with aspects of the present invention. The communication system **5300** includes one or more accessors **5360**, **5362** (also referred to interchangeably herein as one or more "users") and one or more terminals **5342**, **5366**. In one aspect of the present invention, data for use is, for example, input and/or accessed by accessors **5360**, **5364** via terminals **5342**, **5366**, such as personal computers (PCs), minicomputers, mainframe computers, microcomputers, telephonic devices, or wireless devices, such as personal digital assistants ("PDAs") or a hand-held wireless devices coupled to a server **5343**, such as a PC, minicomputer, mainframe computer, microcomputer, or other device having a processor and a repository for data and/or connection to a repository for data, via, for example, a network **5344**, such as the Internet or an intranet, and couplings **5345**, **5346**, **5364**. The couplings **5345**, **5346**, and **5364** include, for example, wired, wireless, or fiberoptic links. In another aspect of the present invention, the method and system of the present invention operate in a stand-alone environment, such as on a single terminal.

[0282] Example aspects have now been described in accordance with the above advantages. It will be appreciated that these examples are merely illustrative hereof. Many variations and modifications will be apparent to those skilled in the art.

What is claimed is:

1. A radiopharmaceutical production system comprising:  
a synthesis unit comprising a plurality of separate synthesis components; and

a connection receiving active product from a radionuclide generator,

wherein each of the synthesis components is configured to individually produce at least one radiopharmaceutical product comprising the received active product.

2. The system according to claim 1, further comprising:

a splitter positioned between the connection and the synthesis unit, wherein the splitter comprises:

a vessel for receiving the active product; and

a synthesis unit selector that directs a predetermined amount of the received active product to at least one of the synthesis components.

3. The system according to claim 2, wherein the splitter further comprises:

a pump positioned between the vessel and the synthesis unit selector, wherein the pump pumps the predetermined amount of active material from the vessel to the synthesis unit selector.

4. The system according to claim 3, wherein the splitter further comprises:

a prime loop connected between the vessel and the pump;

a line between the pump and synthesis unit selector;

a rinse fluid line comprising a connection to the pump that enables a rinse fluid to be pumped through at least a portion of the prime loop; and

a gas supply line, wherein the fluid line and the gas line comprise a connection to the pump that enables a gas to be pumped through at least the line between the pump and the synthesis unit selector.

5. The system according to claim 4, wherein the pump comprises a two position pump, wherein at a first position, the pump:

connects a first portion and a second portion of the prime loop; and

connects the gas line to the line between the pump and the synthesis unit selector, and

wherein in a second position, the pump:

disconnects the prime loop,

connects the vessel to the line between the pump and the synthesis unit selector, and

connects the rinse fluid line to the second portion of the prime loop.

6. The system according to claim 1, wherein each of the plurality of synthesis components comprise a module and a cassette that connect to form a synthesis element, wherein the synthesis element comprises a reaction vessel and at least one of a QMA cartridge, heating provisions, a mixing chamber, a neutralizing chamber, a final production collection chamber, and a solid phase exchange cartridge.

7. The system according to claim 6, wherein each of the plurality of synthesis components comprise at least one valveless pressure pump.

8. The system according to claim 7, wherein the valveless pressure pump comprises at least one of a cascade pump and a membrane pump.

9. The system according to claim 7, wherein the synthesis component further comprises a reagent component comprising a reagent material used to produce the radiopharmaceutical product from the active product.

10. The system according to claim 9, wherein the reagent component is removable from the synthesis component.



**11.** The system according to claim 6, wherein each of the synthesis components comprises a modular synthesis component that is configured to be interchangeable with any of the other synthesis components.

**12.** The system according to claim 11, wherein the synthesis unit comprises six modular synthesis components.

**13.** The system according to claim 1, further comprising:  
a high performance liquid chromatography (HPLC) unit that performs purification during production of the radiopharmaceutical product from the active product.

**14.** The system according to claim 13, wherein the HPLC unit comprises a modular HPLC unit having a plurality of columns and a column selector device.

**15.** The system according to claim 14, wherein the columns are disposable.

**16.** The system according to claim 14, wherein the HPLC unit connects to at least one of the synthesis components.

**17.** The system according to claim 1, further comprising:  
a splitter;  
a purifying component;  
an output component;  
a vial filler;  
a quality control component; and

a sensor that measures at least one of an activity level of a sample and a volume of the sample, wherein the sensor is comprised in at least one of the splitter, the synthesis unit, the purifying component, the output component, the vial filler, and the quality control component.

**18.** The system according to claim 17, wherein the sensor comprises a cadmium zinc telluride (CZT) element.

**20.** The system according to claim 18, wherein the sensor comprises a CZT rod that inserted into the sample.

**21.** The system according to claim 18, wherein the sensor comprises a first CZT element provided at a first column end of a sample column and a second CZT element provided at an opposite column end of the sample column.

**22.** The system according to claim 17, further comprising:  
an analog to digital (A/D) converter that separates pulses according to a height of each pulse measured at the sensor; and

a processing component comprised in a field programmable gate array that converts a signal received from the A/D converter into an activity measurement for the sample.

**23.** The system according to claim 17, further comprising:  
a sample vessel;  
a shield surrounding the sample vessel;  
a probe placed at a side of the sample having the shield interposed between the probe and the sample; and  
a strain gauge positioned below the shield, wherein the shield comprises an opening that enables a portion of the sample vessel to make contact with the strain gauge, wherein the strain gauge determines a volume of the sample based on a strain measurement.

**24.** The system according to claim 1, further comprising an automated, closed path vial filler, the vial filler comprising:

a bulk product vial containing a bulk product;  
a peristaltic pump coupled with the bulk product vial;  
a dispensing manifold assembly coupled with the peristaltic pump; and

at least one final product vial coupled to the dispensing manifold assembly, wherein the peristaltic pump is configured to transfer a predetermined amount of bulk prod-

uct from the bulk product vial to the at least one final product vial via the dispensing manifold assembly.

**25.** The system according to claim 24, the vial filler further comprising:

a stepper motor operably coupled with the peristaltic pump.

**26.** The system according to claim 25, the vial filler further comprising:

a dilution container having a dilution solution, wherein the dilution container is in fluid communication with the bulk product vial and disposed between the peristaltic pump and the dispensing manifold assembly.

**27.** The system according to claim 1, further comprising:

An automated quality control apparatus for testing of radio-synthesized tracers for at least one selected from a group consisting of particle and color content, filter membrane integrity, pH value, residual solvent volume, Kryptofix concentration, bacterial endotoxins concentration, radionuclidic identify, radionuclidic purity, radiochemical identity, radiochemical purity, and sterility.

**28.** The system according to claim 27, wherein the quality control apparatus further stores records of testing results.

**29.** The system according to claim 27, wherein the quality control apparatus performs self calibration

**30.** The system according to claim 27, wherein the quality control apparatus performs a plurality of tests in parallel.

**31.** The system according to claim 1, further comprising:  
an active product generator.

**32.** The system according to claim 31, wherein the active product generator comprises a continuous output active product generator that generates a selected amount of active product on-demand.

**33.** The system according to claim 32, wherein the continuous output active product generator comprises:

a metering pump and a first check valve to control delivery of a metered amount of a fluid containing O-18 atoms to a target cell irradiated by a proton beam, wherein the proton beam converts O-18 to radioactive F-18;

a second check valve coupled to the target cell to control on-demand removal of a portion of the fluid enriched with F-18; and

a gas pressurized switching valve to chase the portion of the fluid enriched with F-18 from the system.

**34.** The system according to claim 33, wherein the continuous output active product generator further comprises:

a reprocessing line that returns unused material for reuse; and

an electrochemical component for separating and cleaning the unused material prior to reuse.

**35.** The system according to claim 1, further comprising an automated labeling component that labels the radiopharmaceutical product.

**36.** The system according to claim 1, further comprising a communication connection to a dispensing pharmacy.

**37.** The system according to claim 36, wherein the dispensing pharmacy is remote from the synthesis unit.

**38.** The system according to claim 1, further comprising a control component that interfaces with the synthesis unit to manage the production of the radiopharmaceutical product.

**39.** The system according to claim 38, wherein the system further comprises a splitter, and wherein the control compo-



nent further comprises an interface for controlling the splitter to manage the production of the radiopharmaceutical product.

**40.** The system according to claim **39**, wherein the system further comprises a vial filler, and wherein the control component further comprises an interface for controlling the vial filler to manage the production of the radiopharmaceutical product.

**41.** The system according to claim **40**, wherein the system further comprises a quality control apparatus, and wherein the control component further comprises an interface for controlling the quality control apparatus to manage the production of the radiopharmaceutical product.

**42.** The system according to claim **41**, wherein the system further comprises a an active product generator, wherein the control component further comprises an interface for controlling the active product generator to manage the production of the radiopharmaceutical product.

**43.** The system according to claim **42**, wherein the system further comprises a labeling component and a connection to a dispensing pharmacy, wherein the control component further comprises an interface for controlling the labeling component and the dispensing pharmacy in order to manage the production and distribution of the radiopharmaceutical product.

**44.** The system according to claim **43**, wherein the control component receives input from a logistics component regarding parameters for the production and distribution of radiopharmaceutical to a patient within a required amount of time and manages the workload of the system based on the received input.

**45.** The system according to claim **43**, wherein the control component generates a report regarding the production of radiopharmaceutical product via the system.

**46.** The system according to claim **43**, wherein the control component tracks pharmaceuticals from a production stage to a patient dosage stage.

**47.** The system according to claim **38**, wherein the control component comprises:

a user interface that receives a selection of a synthesis unit component and receives at least one of a type and an amount of radiopharmaceutical product to be produced, wherein the control component operates the system in order to produce the amount of radiopharmaceutical received via the user interface and using the indicated synthesis unit component.

**48.** The system according to claim **47**, wherein the user interface further comprises:

a graphic representation of a connection between subcomponents of the system used for production of the indicated radiopharmaceutical product.

**49.** A method of producing radiopharmaceuticals, comprising:

generating radionuclides for use in production of a radiopharmaceutical product;  
receiving instructions via a user interface to produce the radiopharmaceutical product; and  
automatically synthesizing the radiopharmaceutical product using the radionuclides.

**50.** The method of claim **49**, further comprising:  
removing unwanted products included with at least one selected from a group consisting of the generated radionuclides, the radiopharmaceutical, and an intermediate compound in the synthesis.

**51.** The method of claim **49**, further comprising:  
measuring at least one selected from a group consisting of a quantity and an activity level of a sample during the radiopharmaceutical production process.

**52.** The method of claim **49**, further comprising:  
distributively delivering the radionuclides in an appropriate quantity to one of a plurality of modular cassette synthesis units in a modular cassette subsystem for production of radiopharmaceutical output.

**53.** The method of claim **49**, further comprising:  
distributively delivering the radionuclides in appropriate quantities to a plurality of modular cassette synthesis units in a modular cassette subsystem for parallel production of radiopharmaceutical output.

**54.** The method of claim **49**, wherein each modular cassette synthesis is configured to allow disposable replacement of portions of the subsystem.

**55.** The method of claim **52**, further comprising:  
delivering appropriate quantities of non-radionuclide components to the plurality of modular cassette synthesis units as part of the production of radiopharmaceutical output.

**56.** The method of claim **55** further comprising:  
upon production of the radiopharmaceutical output from the plurality of modular cassette synthesis units, measuring at least one selected from a group consisting of the quantity and activity level of a stream of radiopharmaceutical output.

**57.** The method of claim **56**, wherein the measuring is performed via at least one selected from a group consisting of a radioactivity sensor and a dose calibrator.

**58.** The method of claim **55**, further comprising  
upon production of the radiopharmaceutical output from the plurality of modular cassette synthesis units, measuring at least one selected from a group consisting of the quantity and activity level of each of a plurality of streams of radiopharmaceutical output.

**59.** The method of claim **49**, further comprising:  
purifying the radiopharmaceutical output.

**60.** The method of claim **49**, wherein purifying the radiopharmaceutical output comprises removing any unwanted products included with the generated radionuclides including drying or deprotecting at least one selected from a group consisting of the generated radionuclides, the radiopharmaceutical, and an intermediate compound.

**61.** The method of claim **60**, wherein the purifying is at least partially performed in at least one disposable column.

**62.** The method of claim **49**, further comprising:  
distributively dispensing bulk product in one or more sterile vials or manufactured dose containers.

**63.** The method of claim **62**, further comprising:  
automatically labeling a container of the radiopharmaceutical product.

**64.** The method of claim **49**, further comprising:  
automatically producing dose related information for use with the doses.

**65.** The method of claim **49**, further comprising:  
performing automated quality control on one or more extracted samples from the produced radiopharmaceutical output.

**66.** The method of claim **49**, further comprising:  
providing dose information to a remote dispensing pharmacy.

**67.** The method of claim **66**, wherein a dose is determined prior to generating radionuclides, and wherein the amount of radionuclide is generated based on the determined dose, and wherein the dose information provided to the remote dispensing pharmacy comprises the previously determined dose.

**68.** The method of claim **49**, further comprising:

providing at least one selected from a group consisting of software and hardware controls for a plurality of sub-portion operation that enables remote at least one selected from a group consisting of data collection, troubleshooting, communication, and control.

**69.** The method of claim **49**, further comprising:

replacing components for a single run product within an internal shielded opening with multiple subsystems that each enable an individual production run.

**70.** The method of claim **69**, wherein the multiple subsystems are configured to allow parallel production operations.

**71.** The method of claim **49**, comprising running a plurality of steps in a quality control process in an automated manner contemporaneously with a dispensing operation of the method.

**72.** The method of claim **49**, further comprising:

running an automated purification process comprising at least one selected from a group consisting of high performance liquid chromatography (HPLC), low pressure chromatography, flash chromatography, and Sep-Pak purification and isolation processes.

**73.** The method of claim **72**, wherein the automated purification process is run using a disposable column.

\* \* \* \* \*