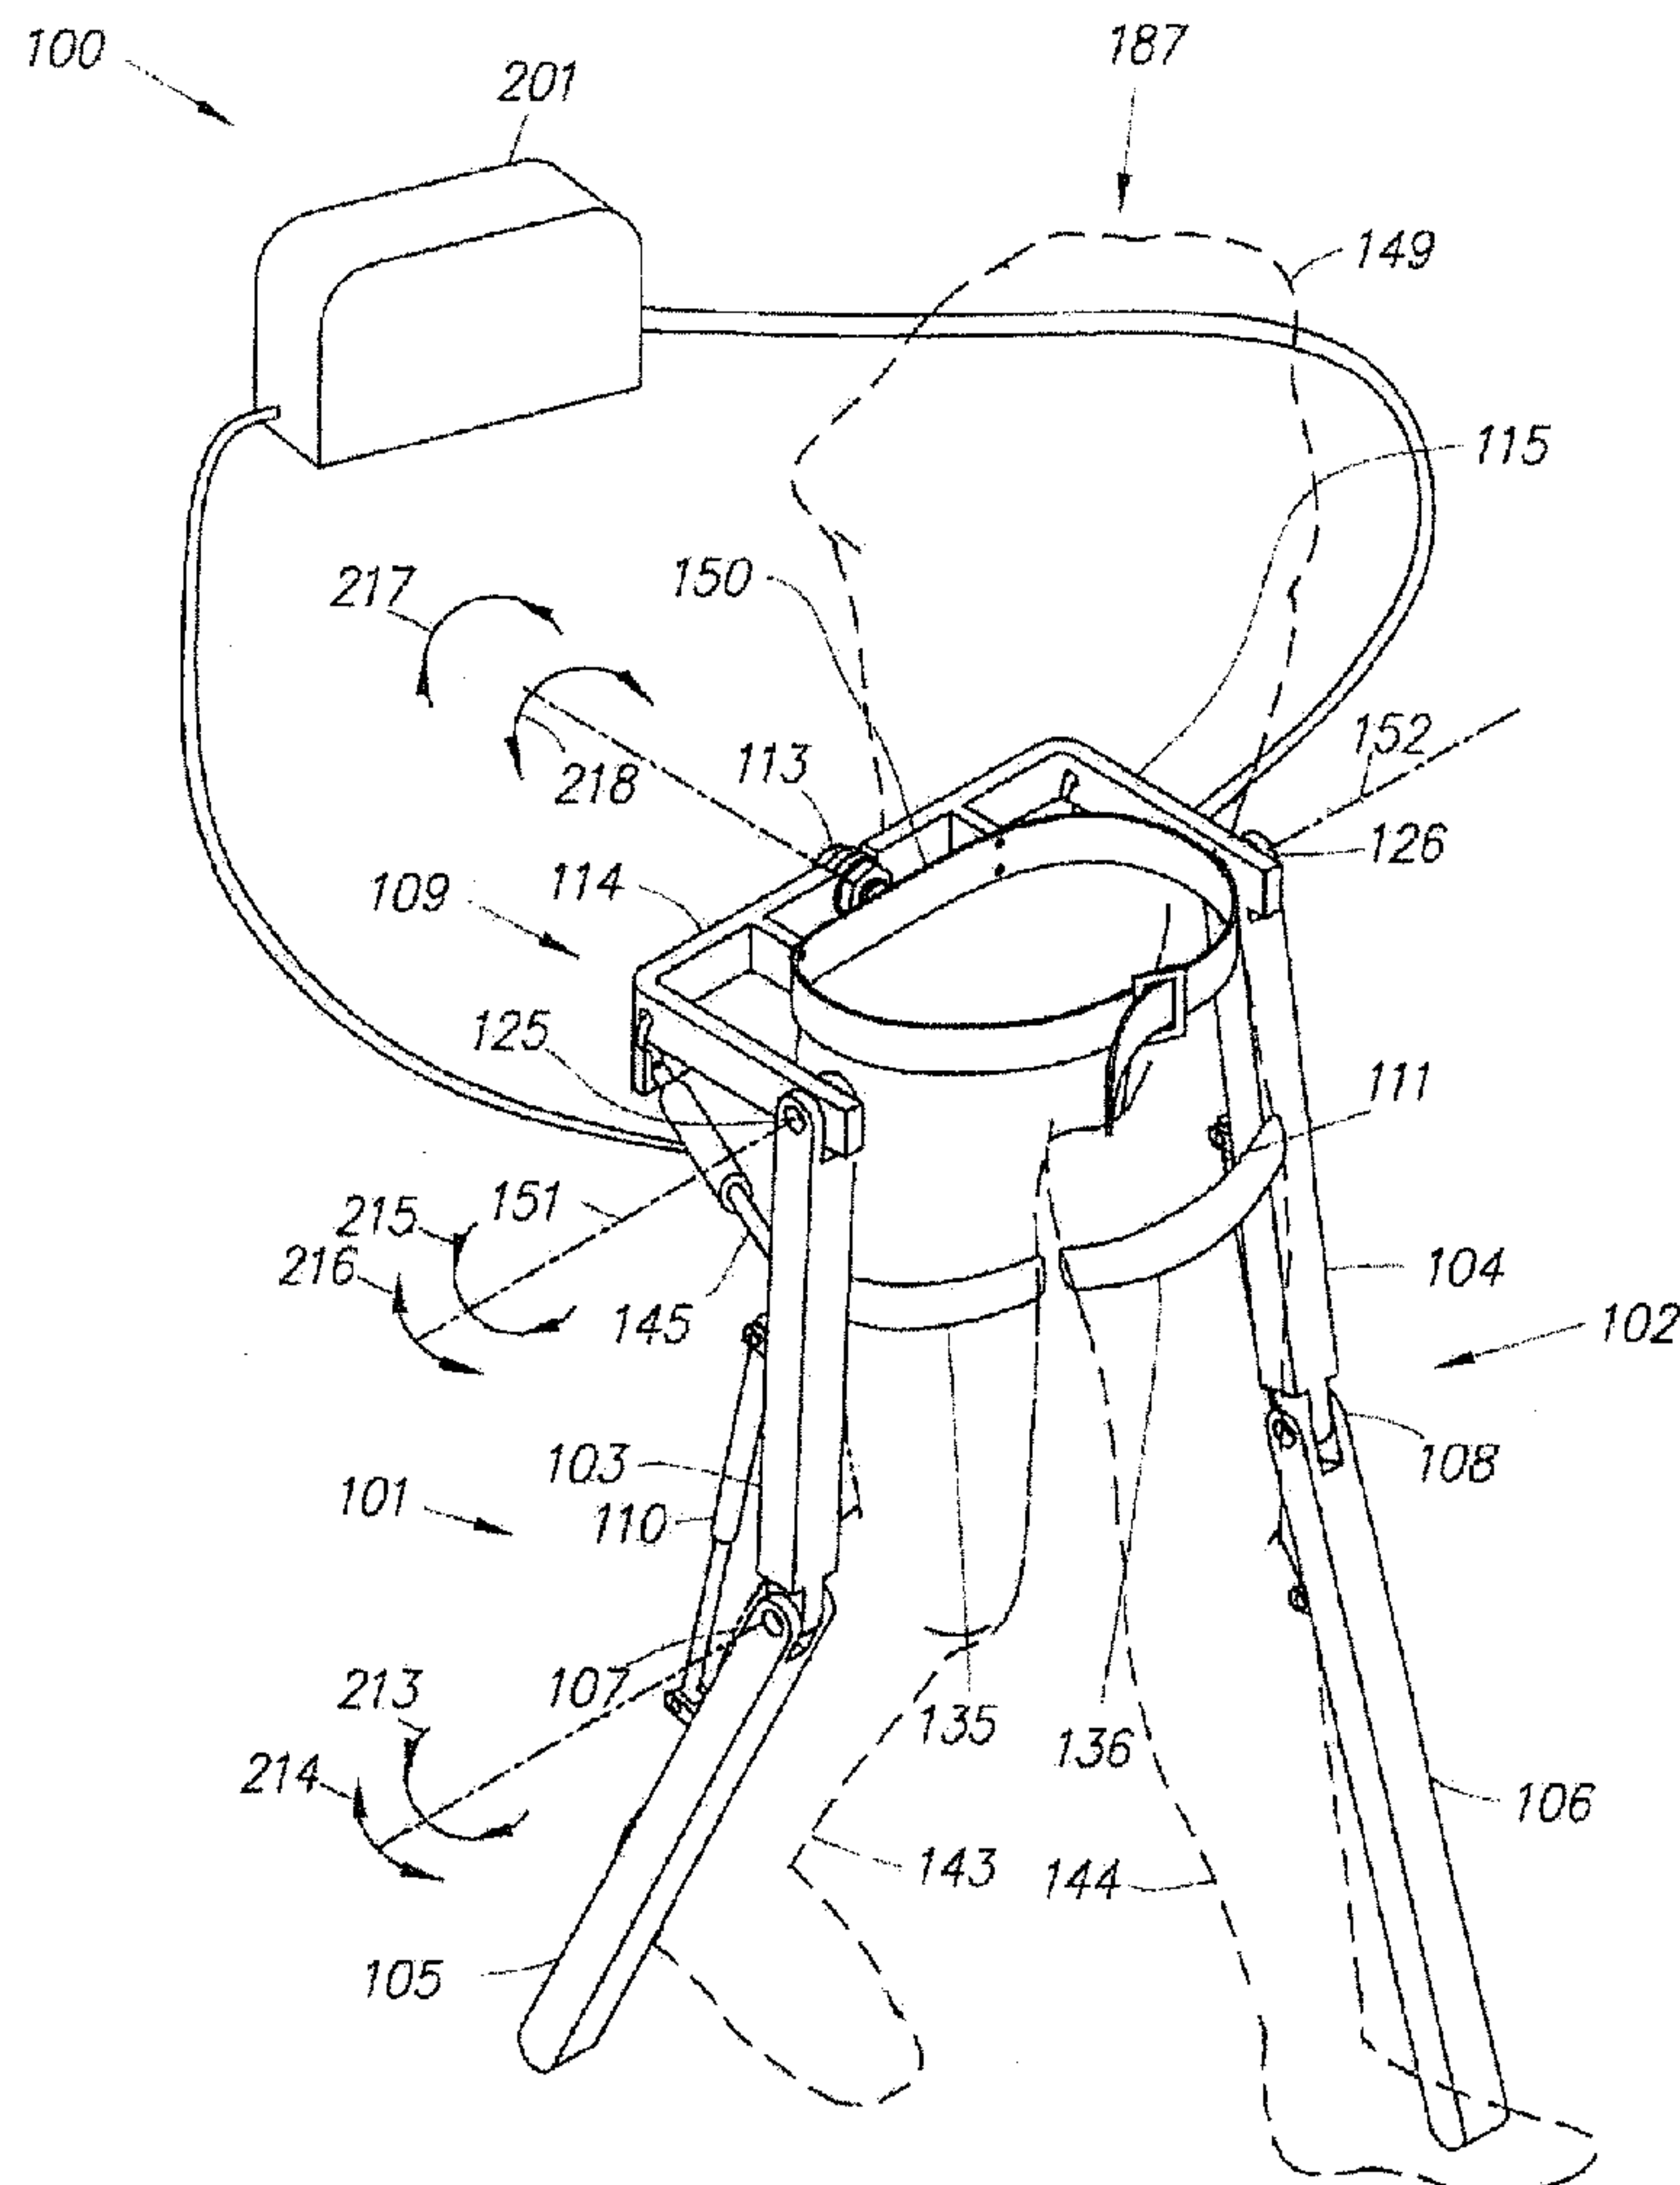


US 20150134078A1

(19) **United States**(12) **Patent Application Publication**
Amundson et al.(10) **Pub. No.: US 2015/0134078 A1**(43) **Pub. Date: May 14, 2015**(54) **DEVICE AND METHOD FOR DECREASING
ENERGY CONSUMPTION OF A PERSON BY
USE OF A LOWER EXTREMITY
EXOSKELETON****Publication Classification**(51) **Int. Cl.**
A61H 3/00 (2006.01)
(52) **U.S. Cl.**
CPC **A61H 3/00** (2013.01)(71) Applicant: **Ekso Bionics, Inc.**, Richmond, CA (US)(72) Inventors: **Kurt Amundson**, Berkeley, CA (US);
Nathan Harding, Oakland, CA (US);
Homayoon Kazerooni, Berkeley, CA
(US)(73) Assignee: **Ekso Bionics, Inc.**, Richmond, CA (US)(21) Appl. No.: **14/605,343**(22) Filed: **Jan. 26, 2015****Related U.S. Application Data**(63) Continuation of application No. 12/468,595, filed on
May 19, 2009, now Pat. No. 8,945,028.(60) Provisional application No. 61/071,823, filed on May
20, 2008.(57) **ABSTRACT**

A lower extremity exoskeleton, configurable to be coupled to a person, includes: leg supports configurable to be coupled to the person's lower limbs and designed to rest on the ground during stance phases, with each leg support having a thigh link and a shank link; two knee joints, each configured to allow flexion and extension between respective shank and thigh links; an exoskeleton trunk configurable to be coupled to the person's upper body, rotatably connectable to the thigh links of the leg supports, allowing for the flexion and extension between the leg supports and the exoskeleton trunk; two hip actuators configured to create torques between the exoskeleton trunk and the leg supports; and at least one power unit capable of providing power to the hip actuators. In use, power is supplied to the hip actuators in an amount to reduce the energy consumed by a user during a walking cycle.



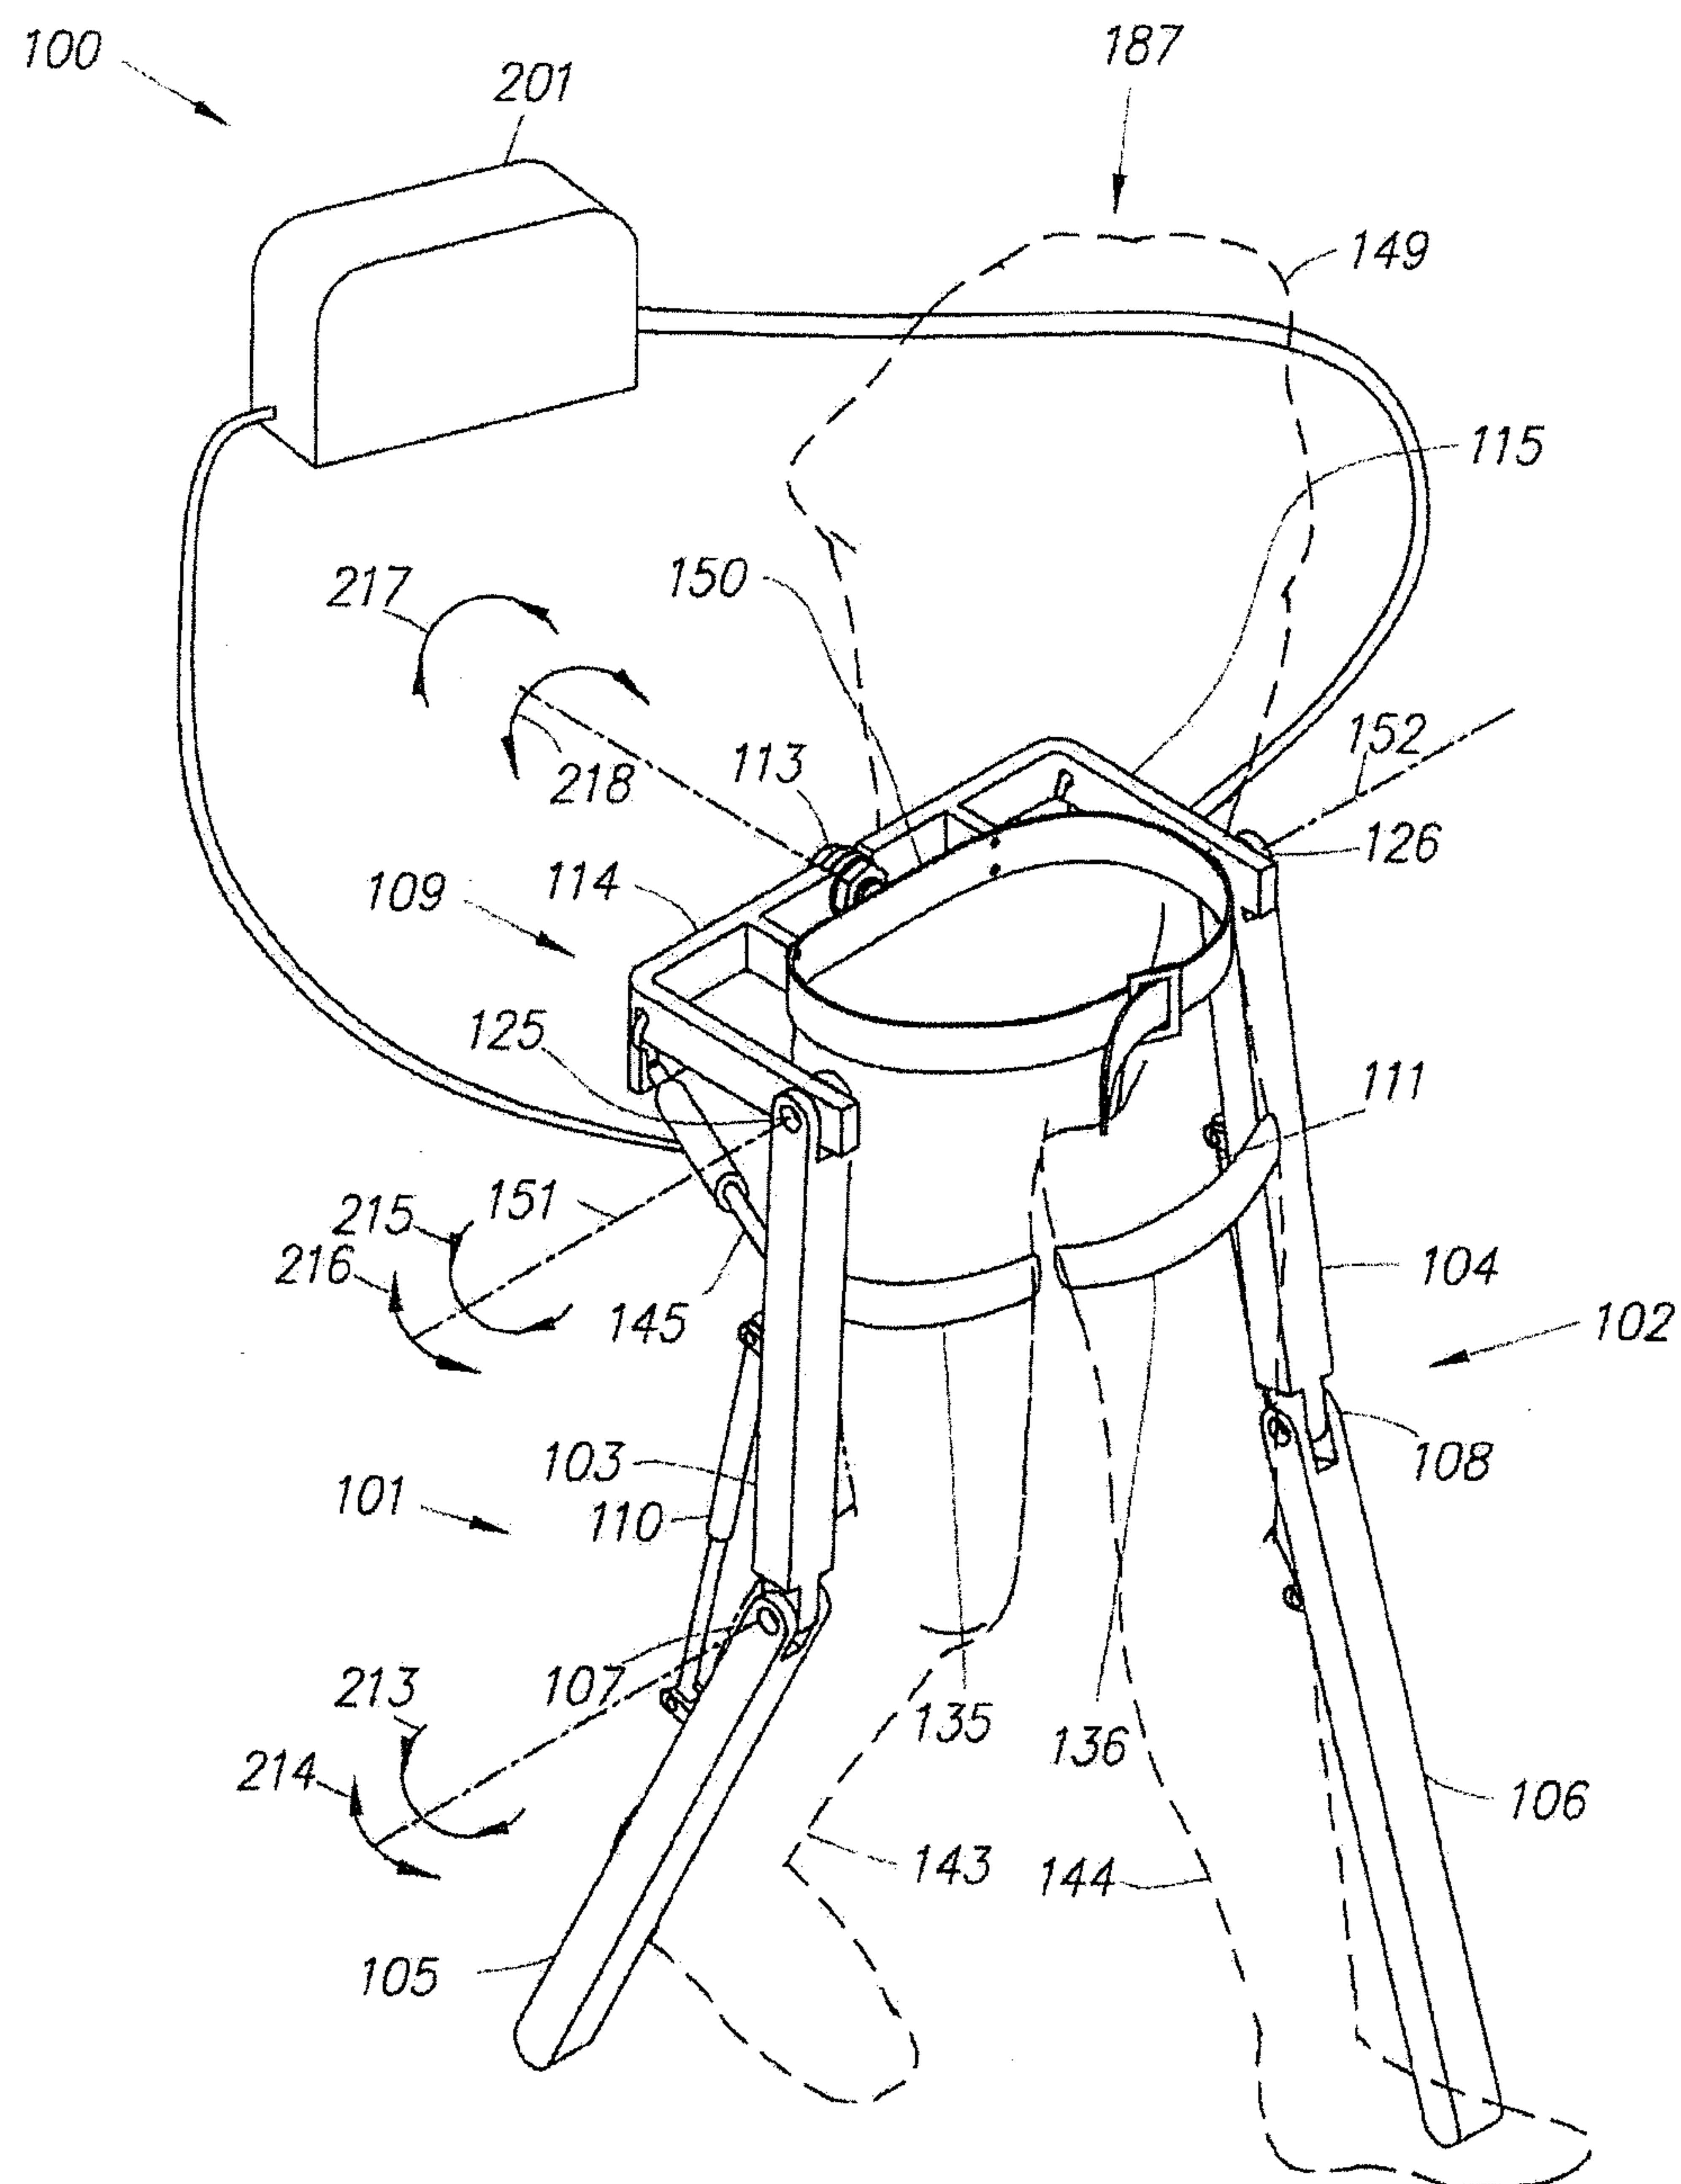


Fig. 1

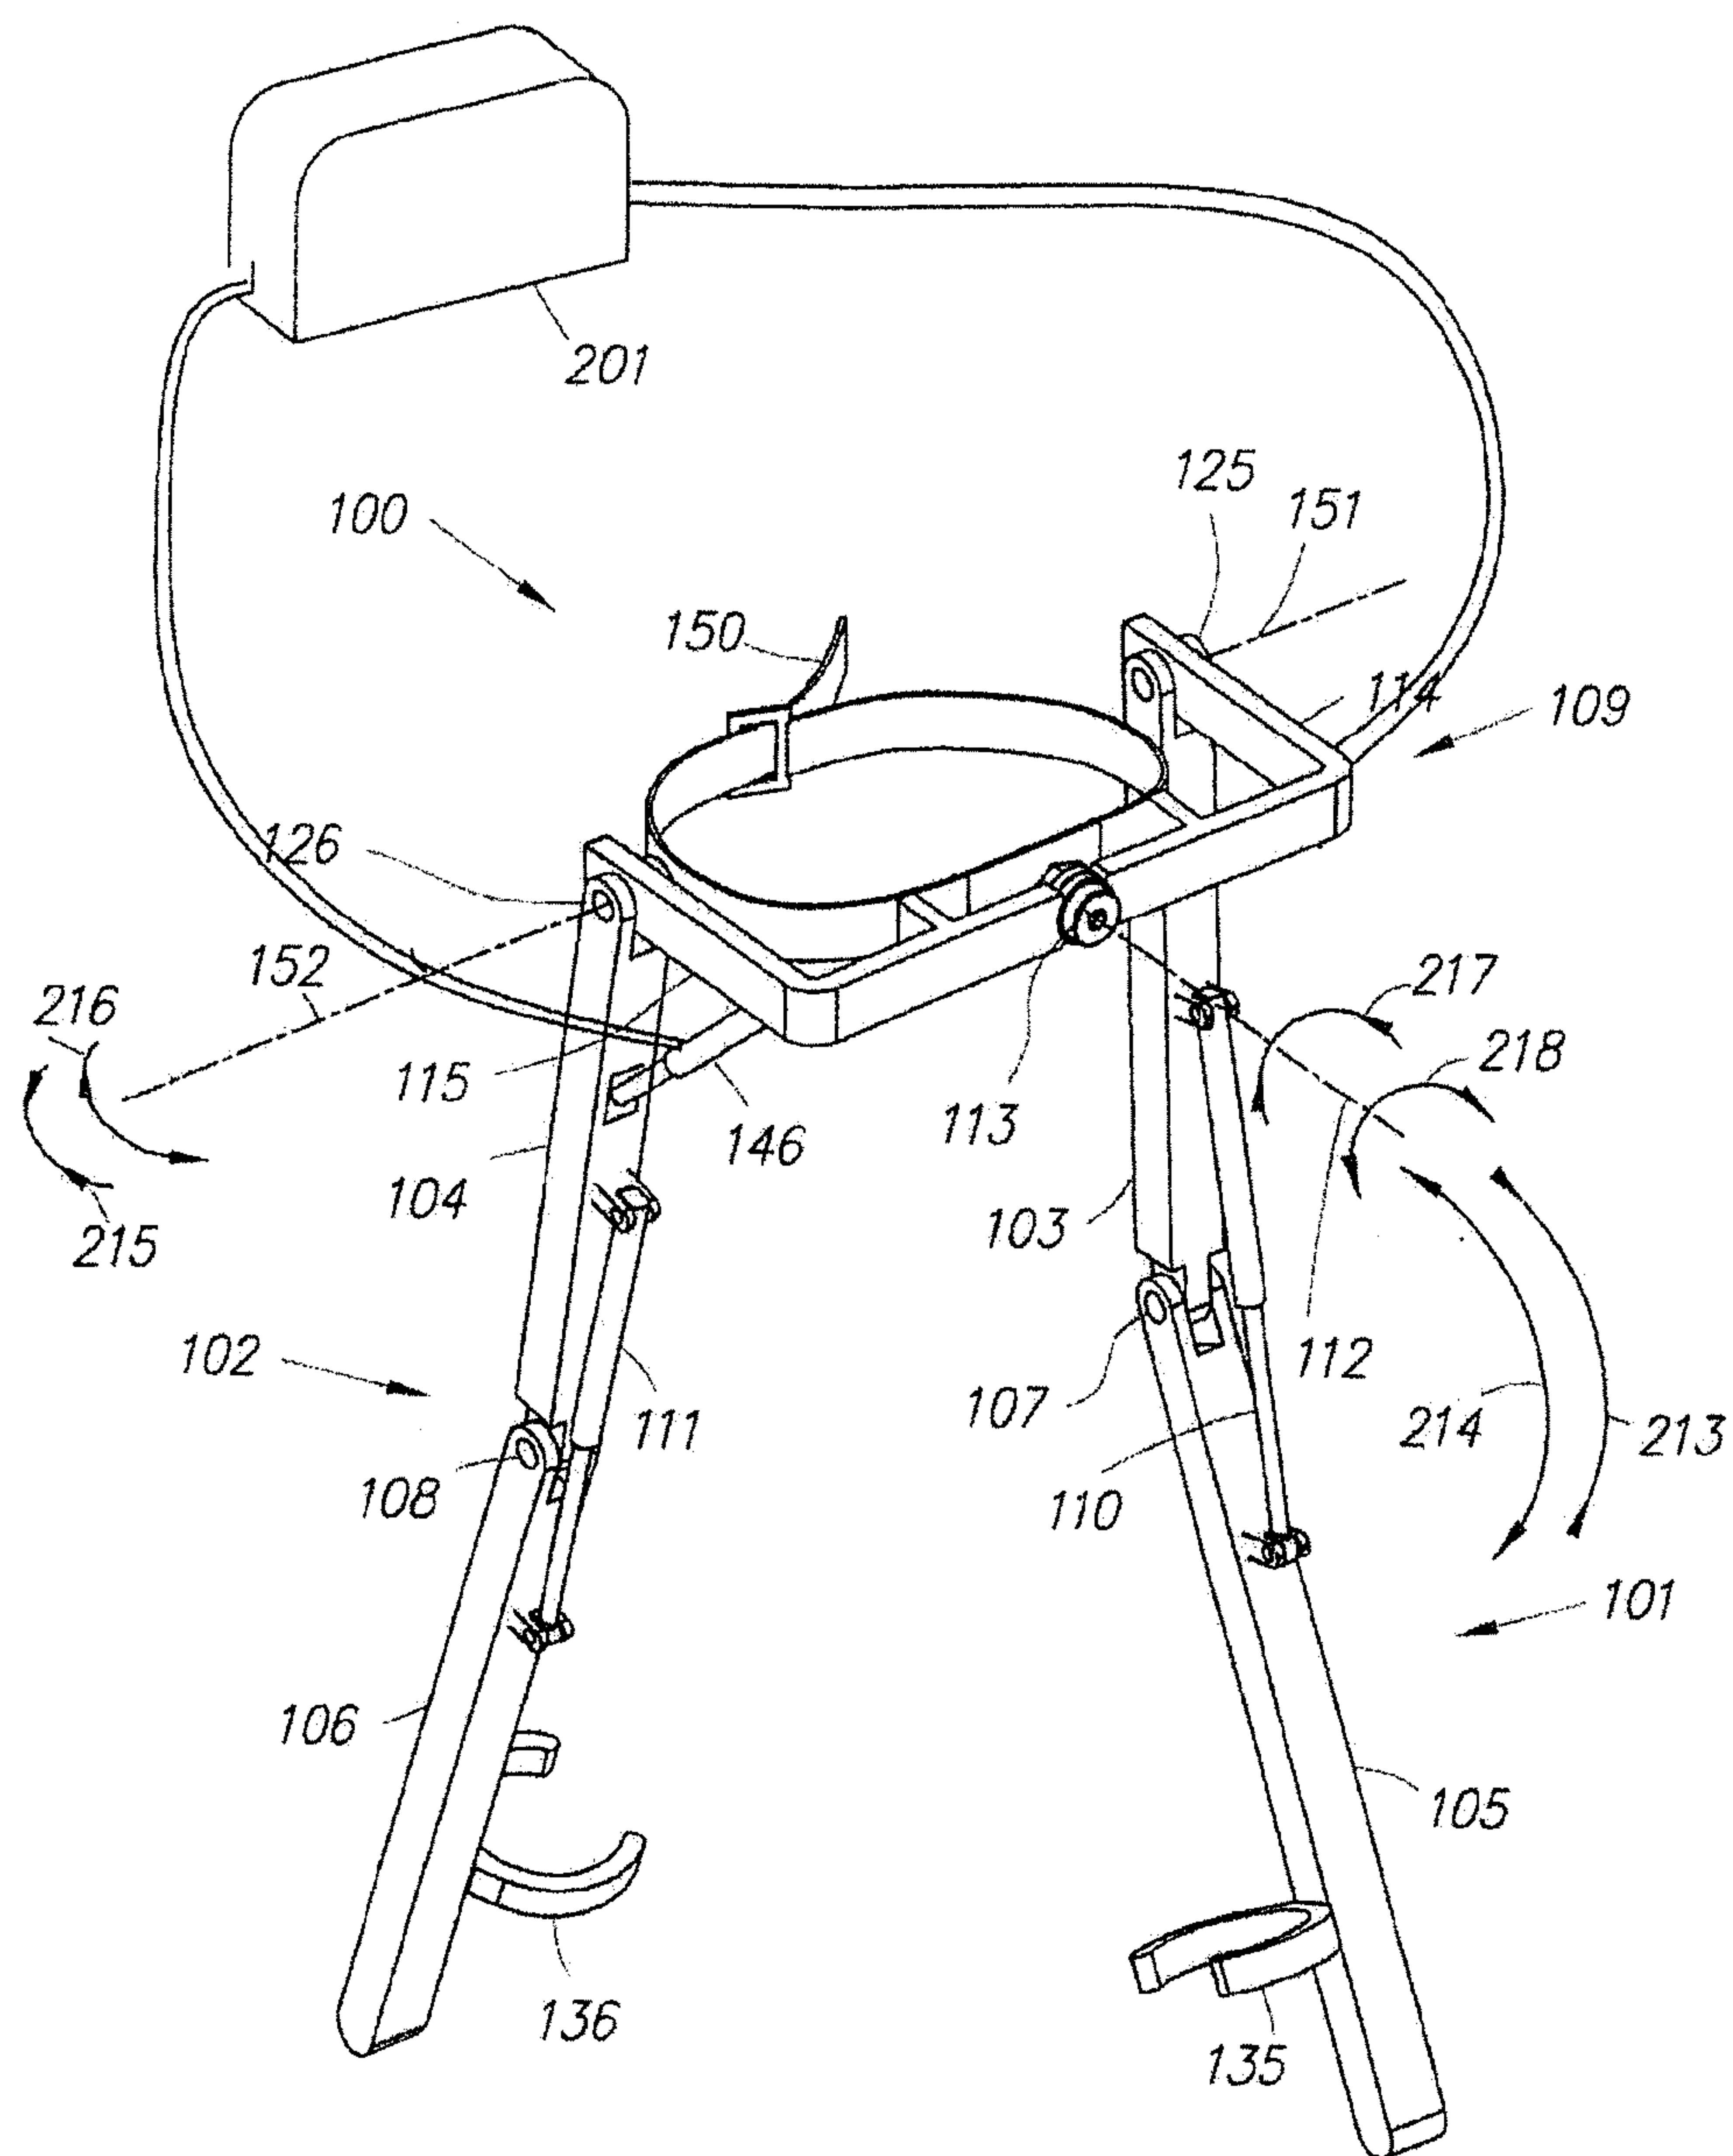
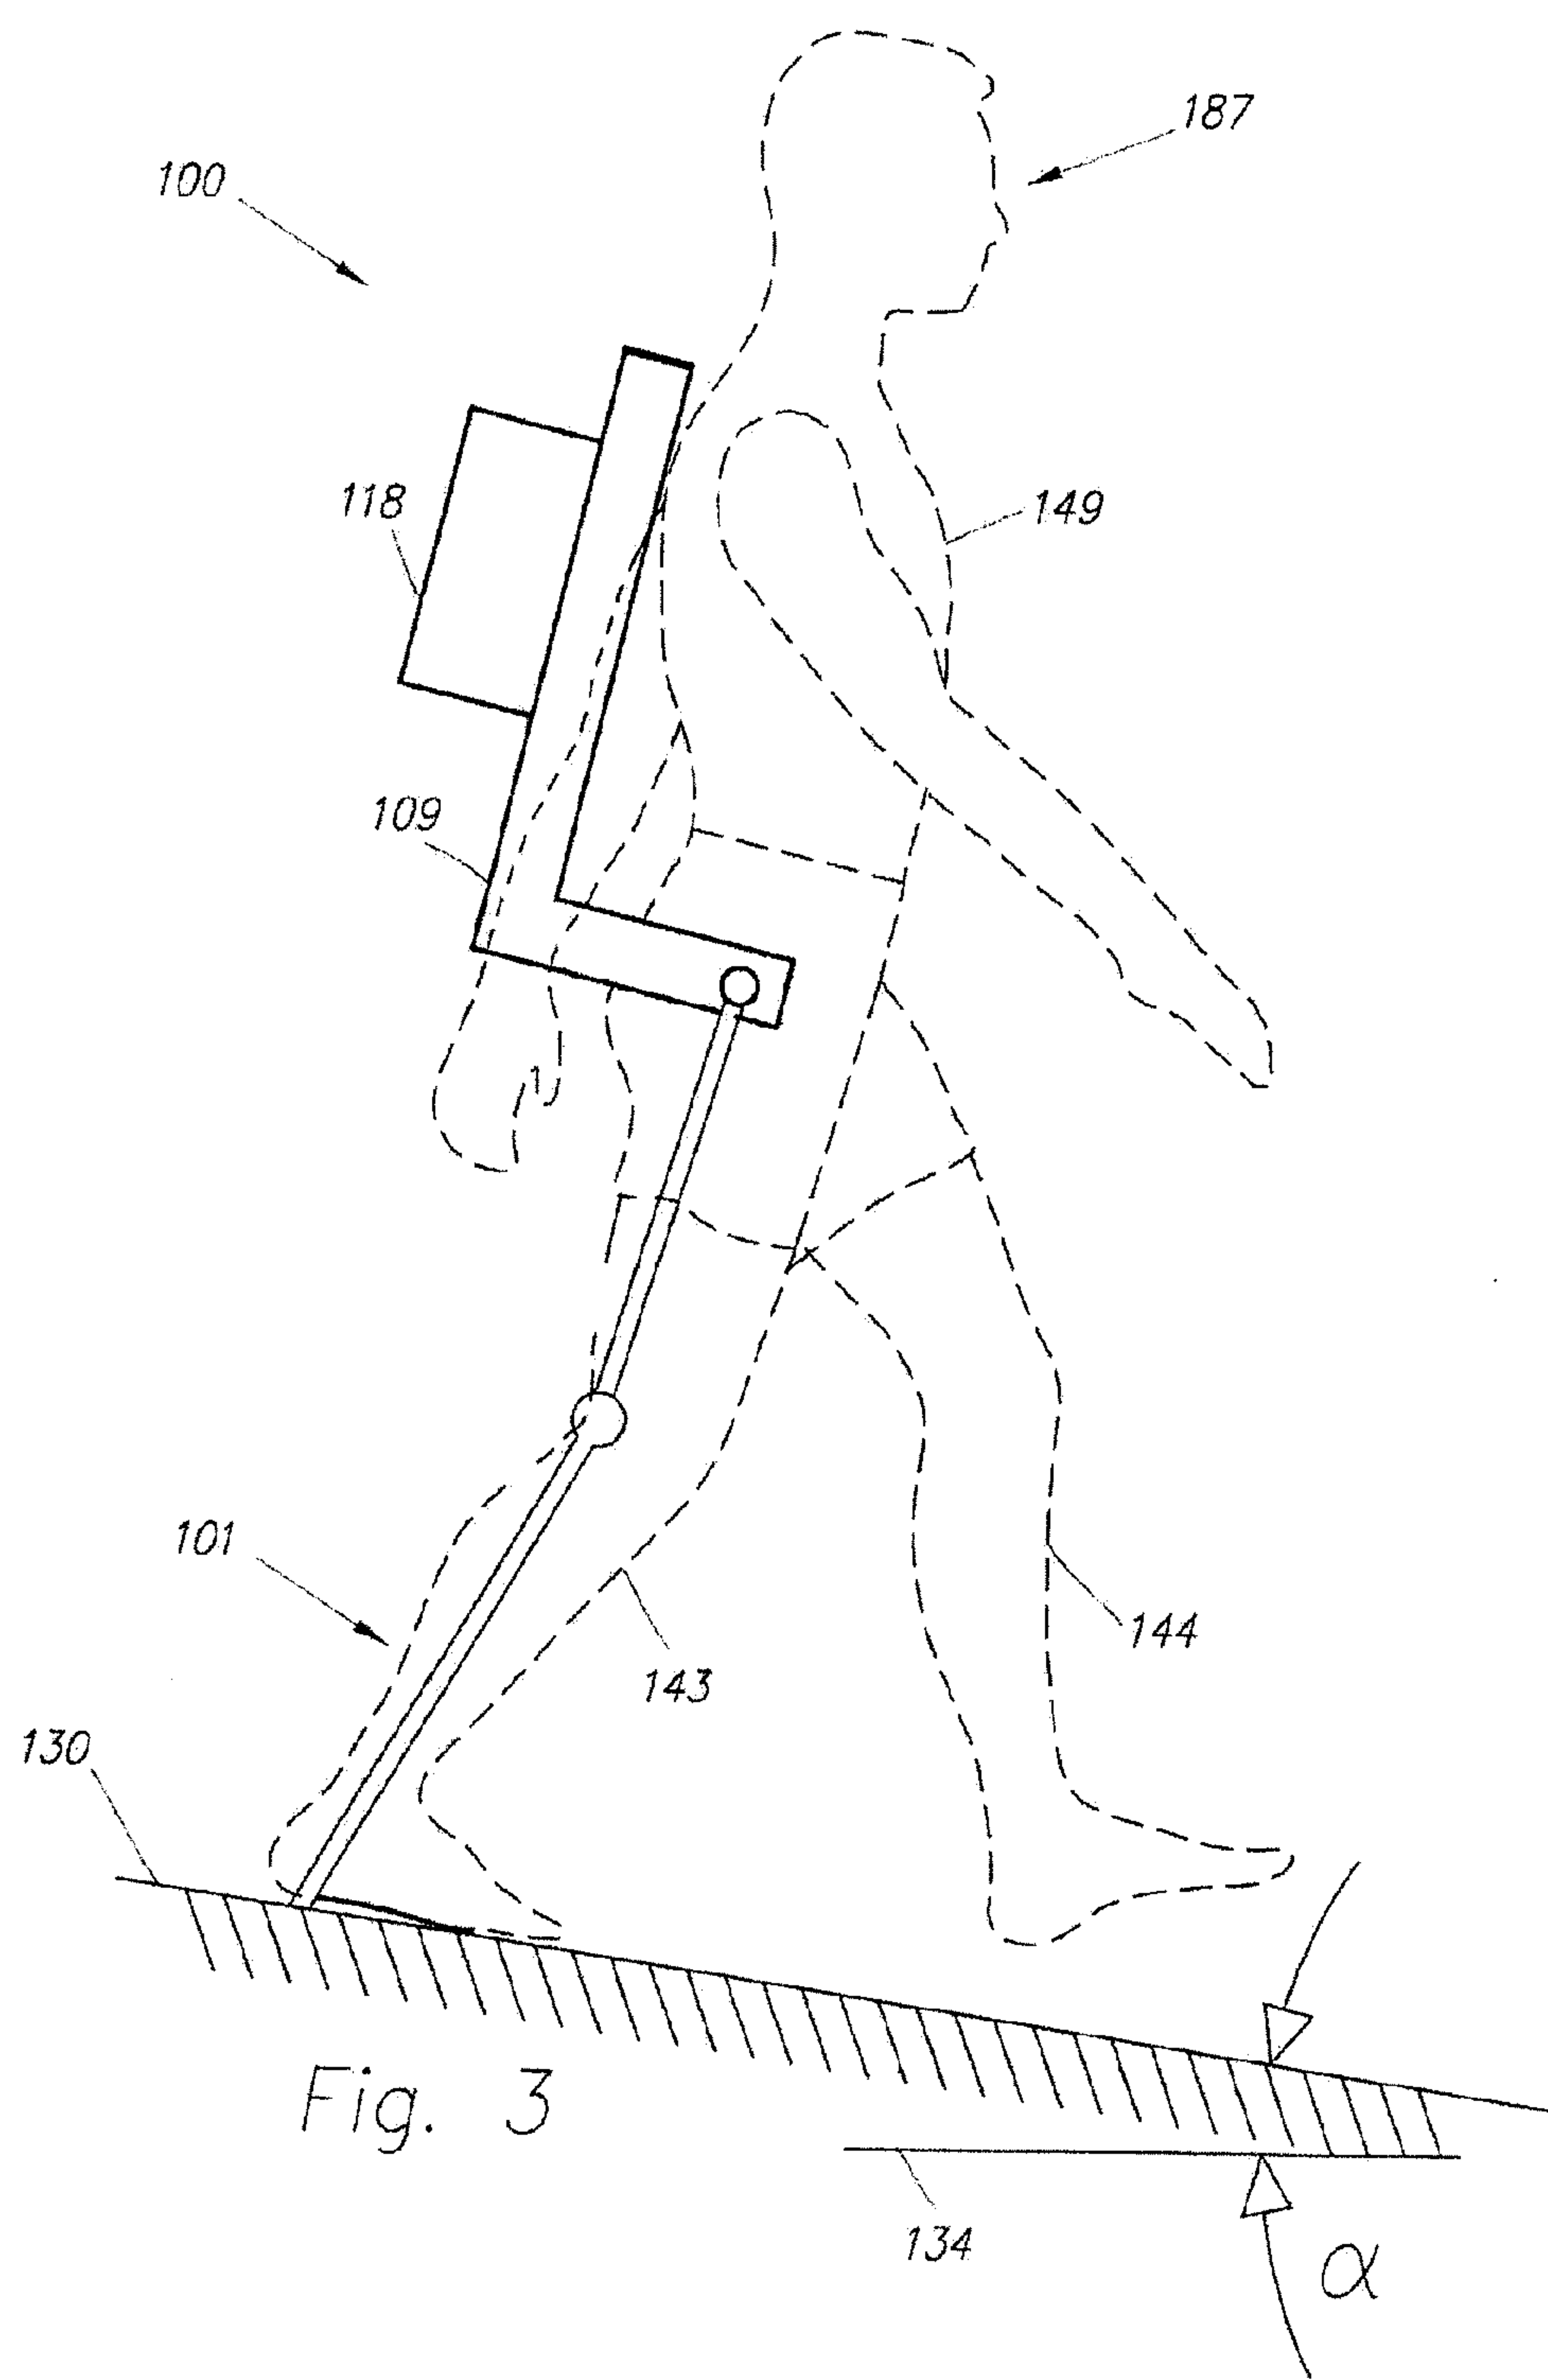


Fig. 2



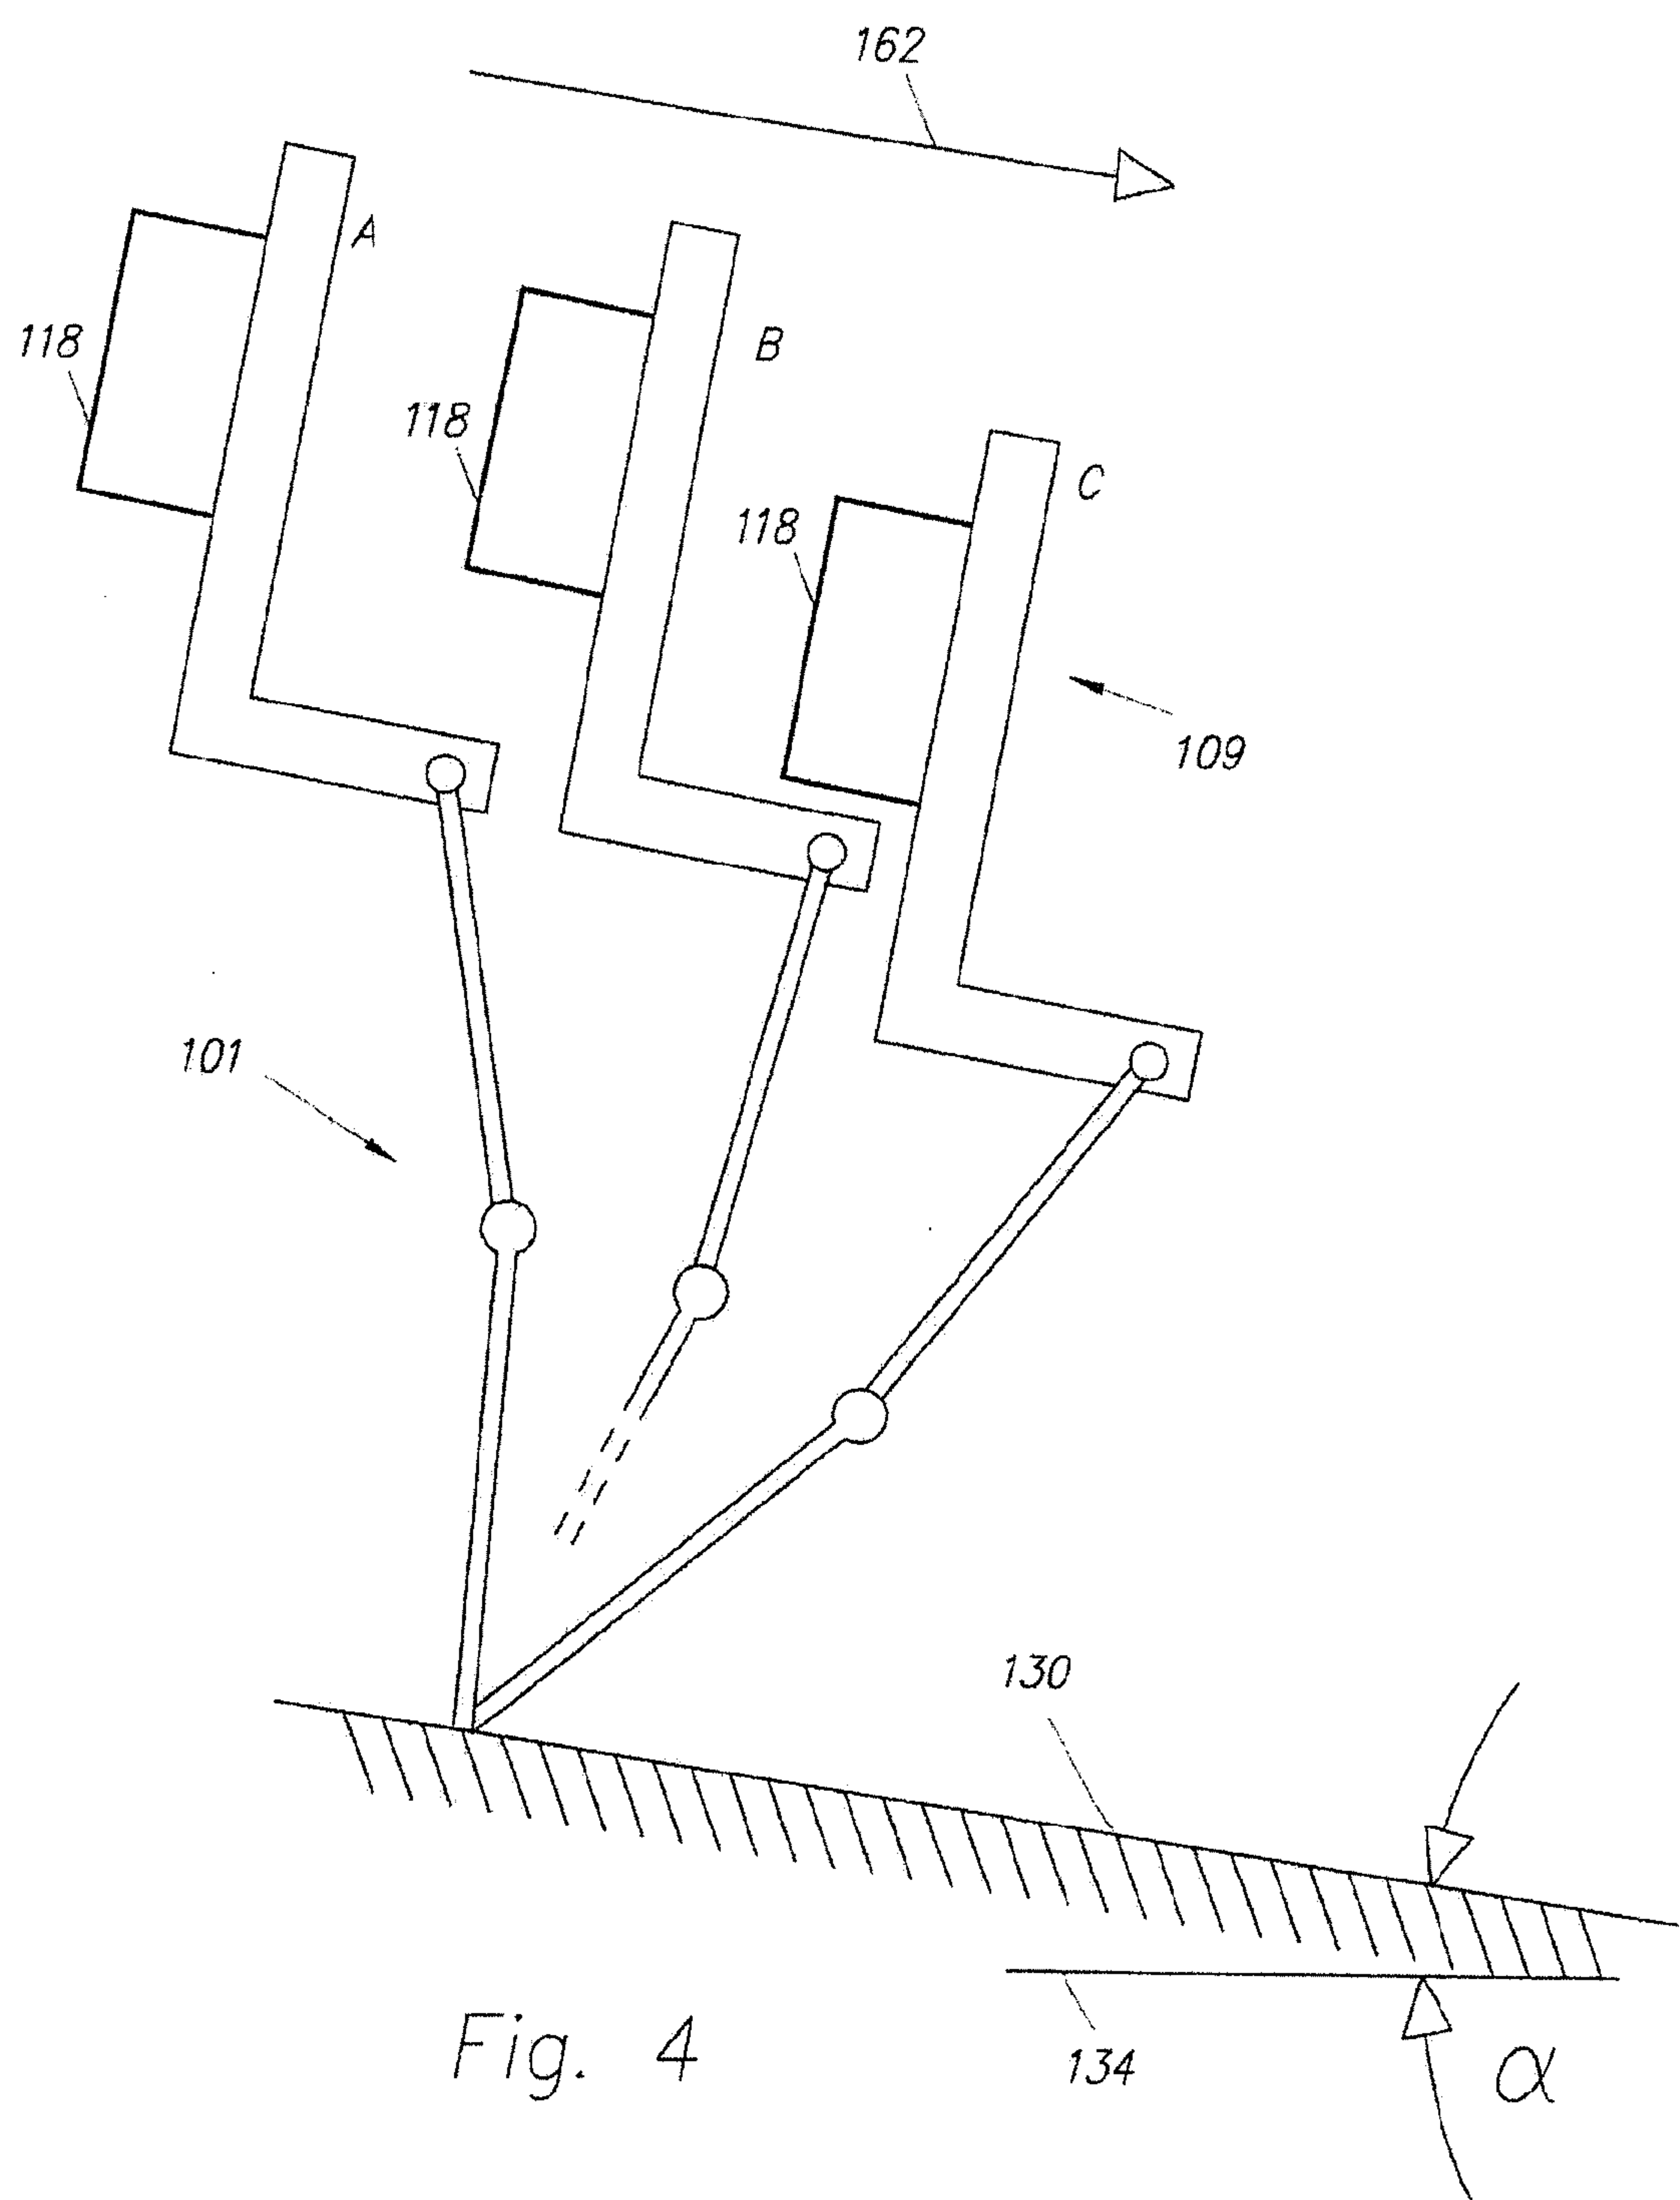
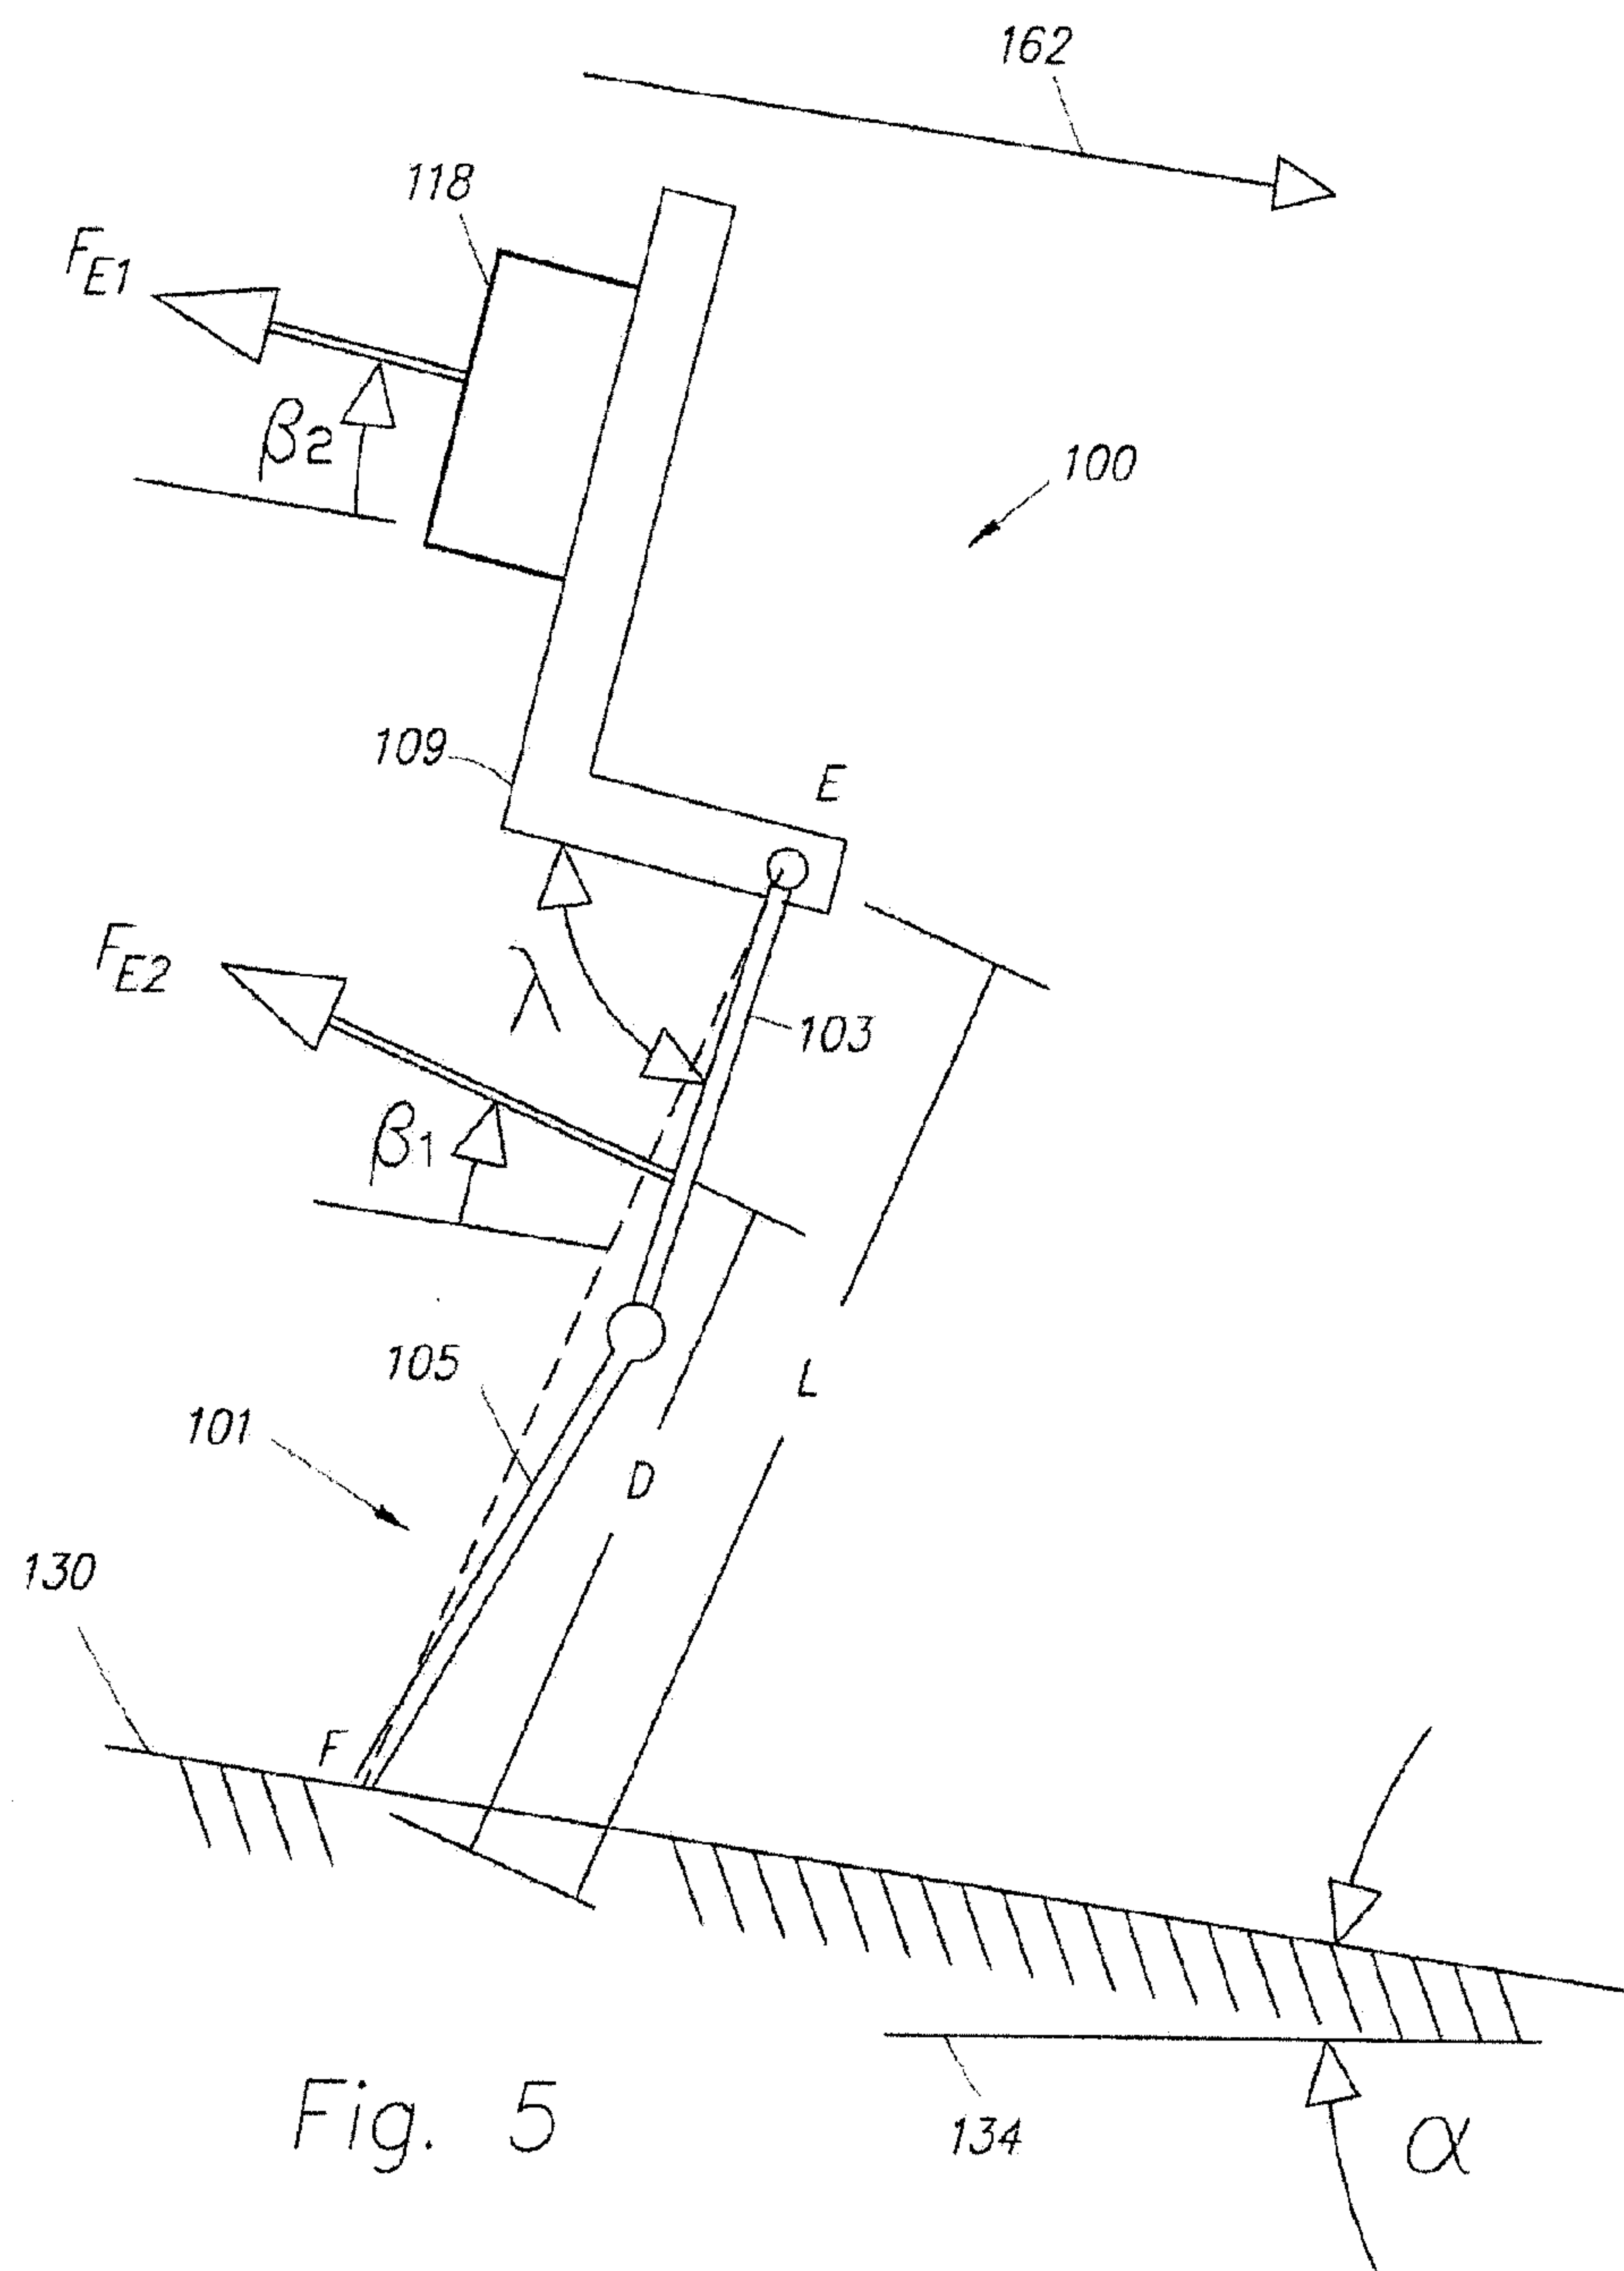


Fig. 4



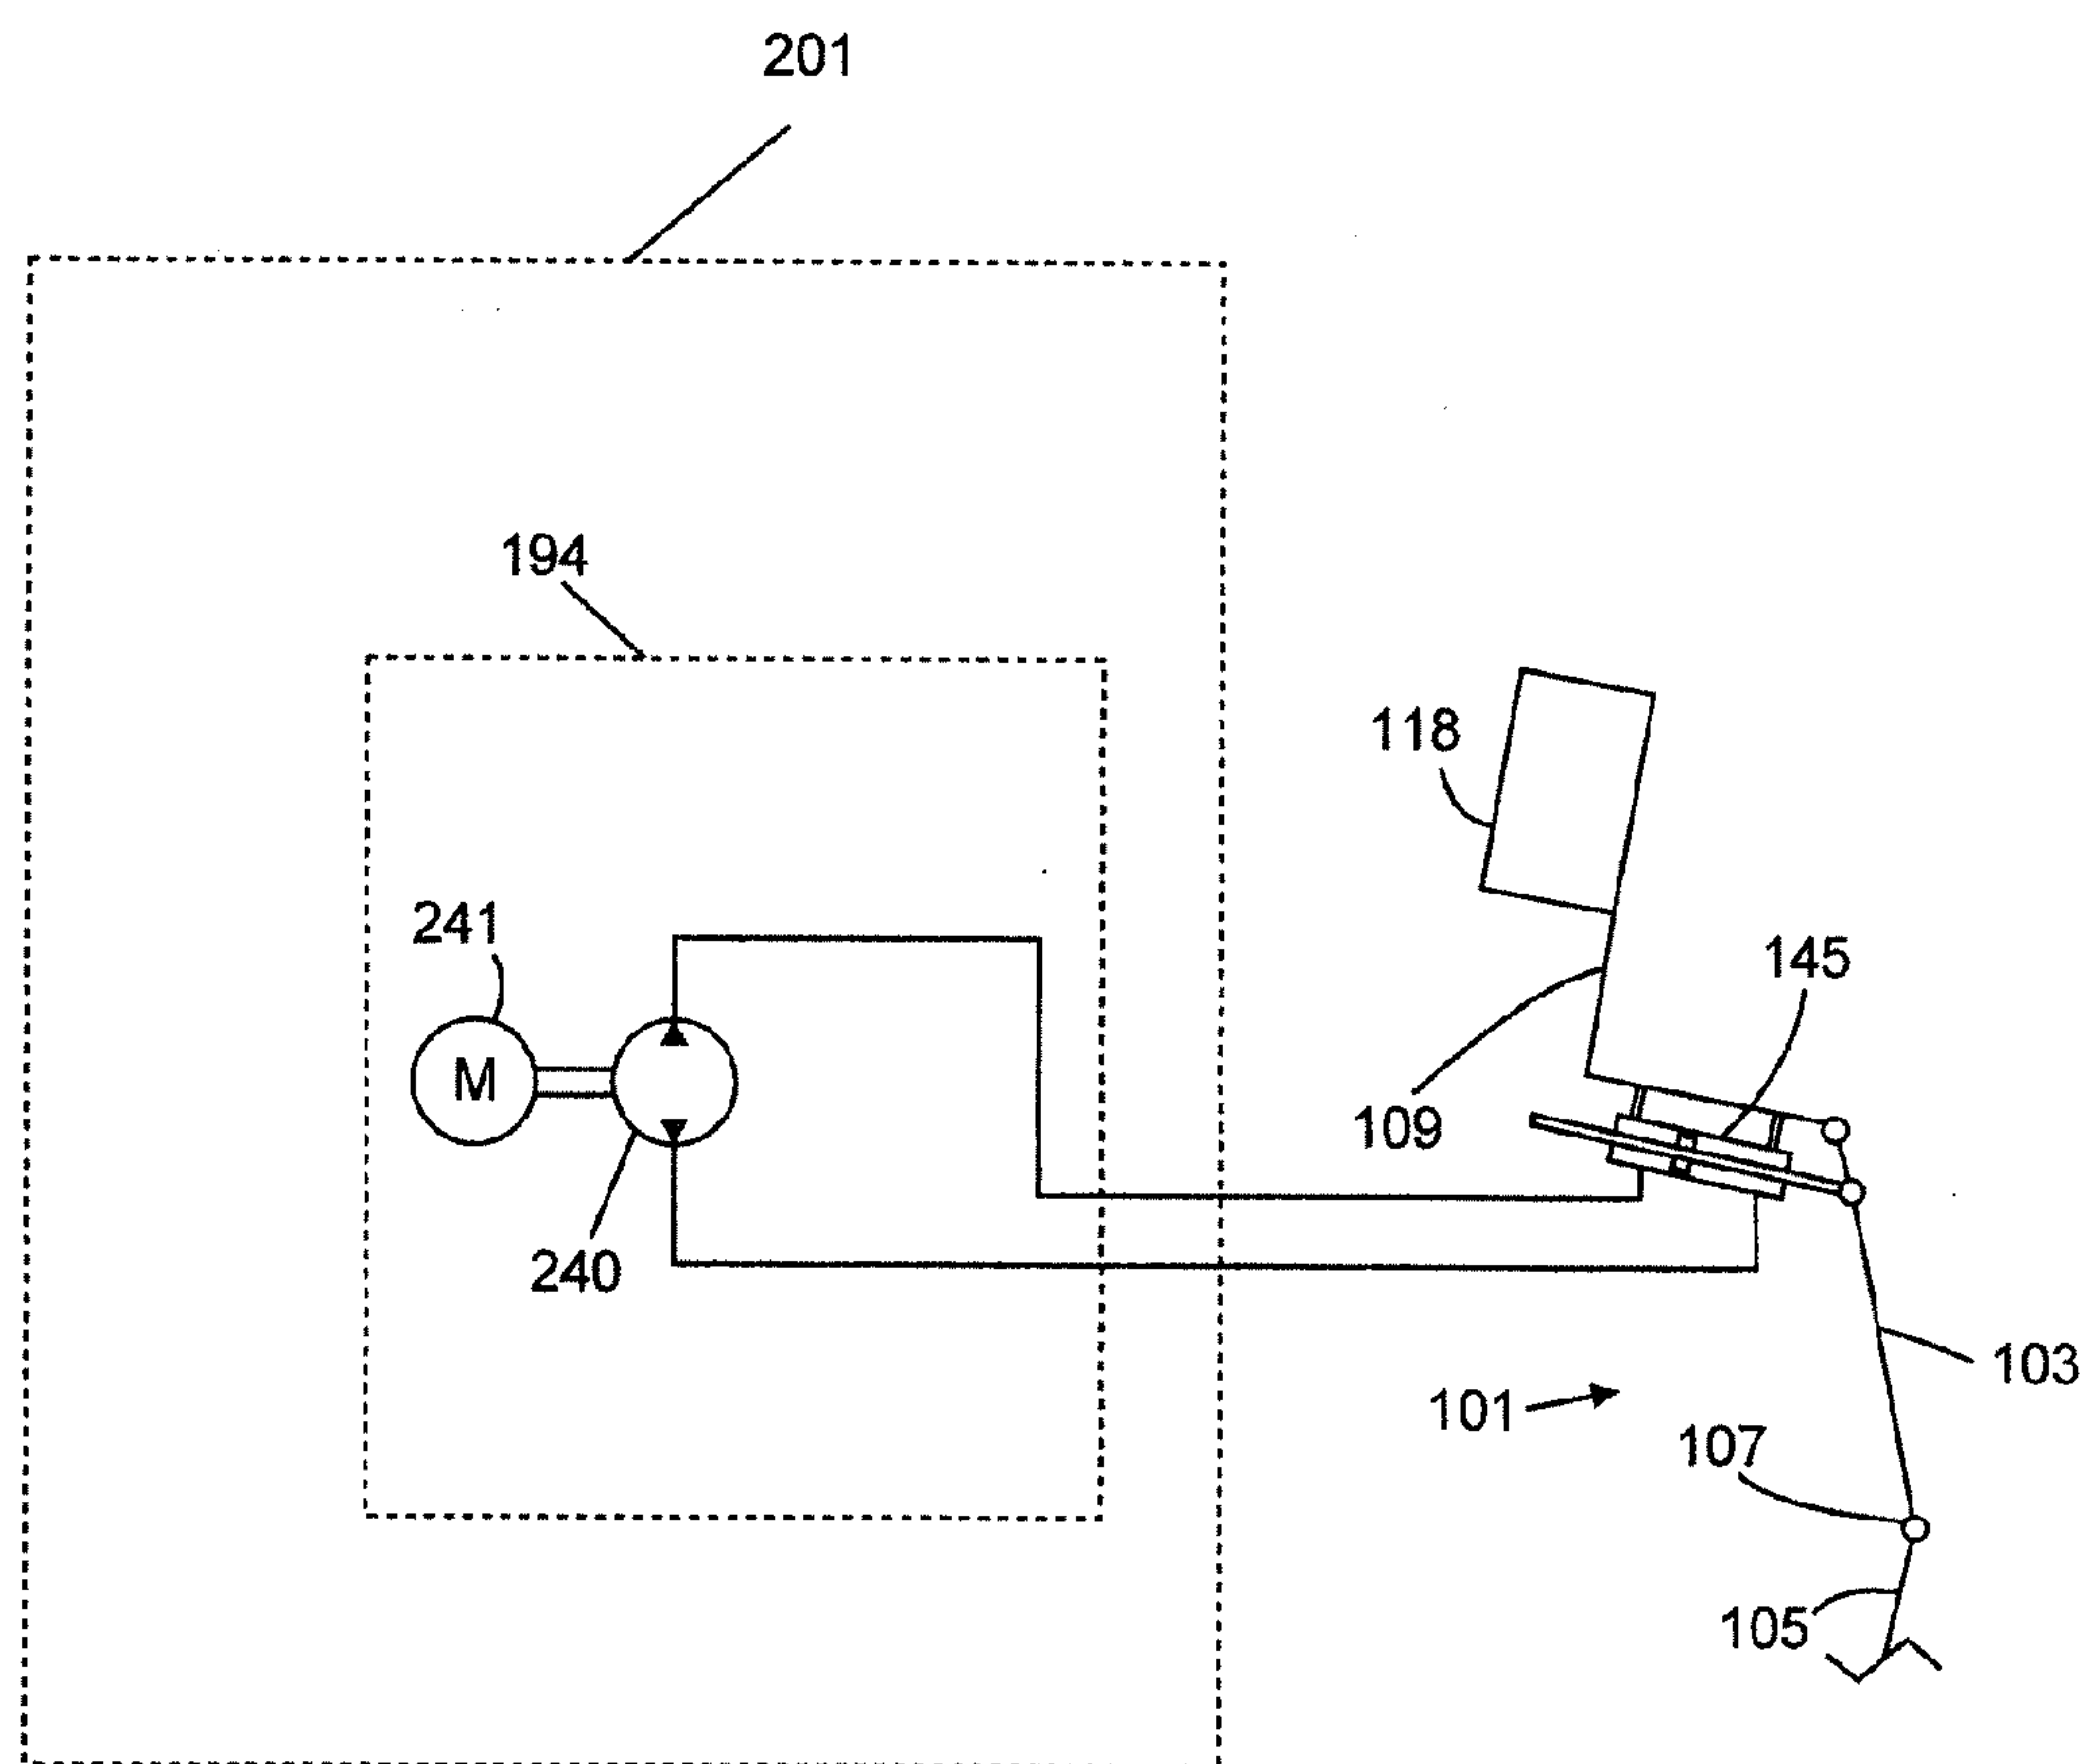


Figure 6

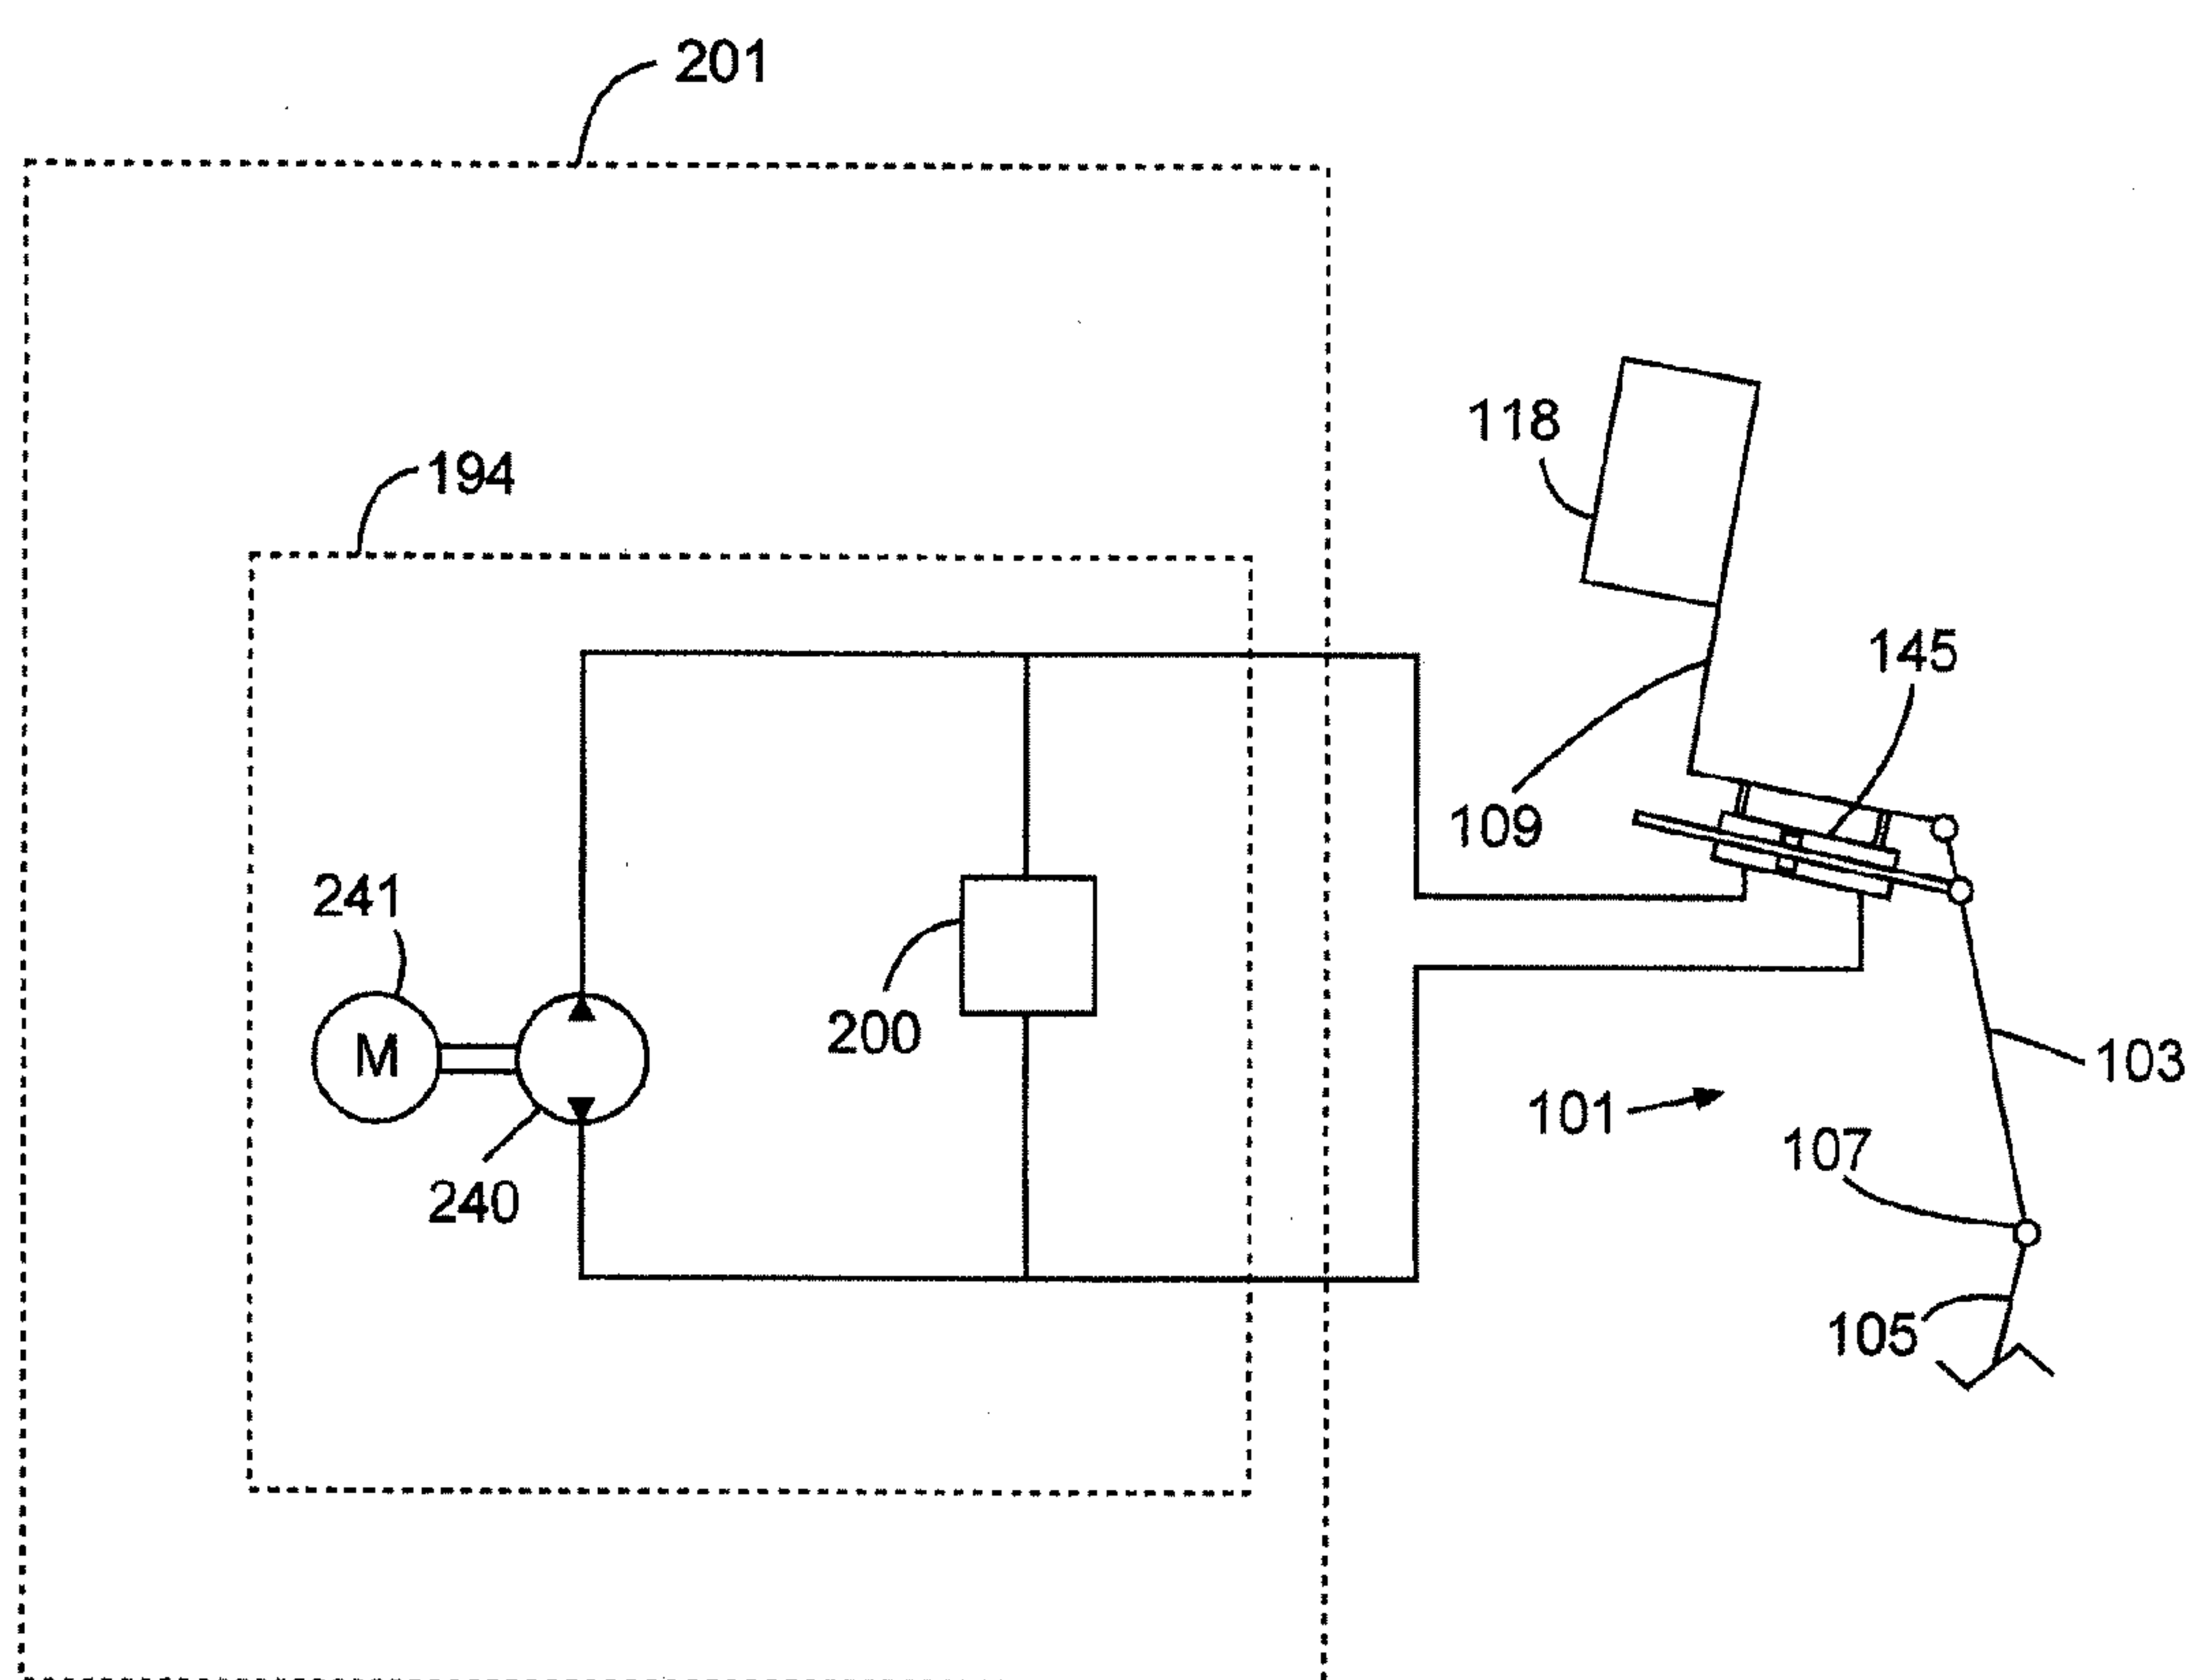


Figure 7

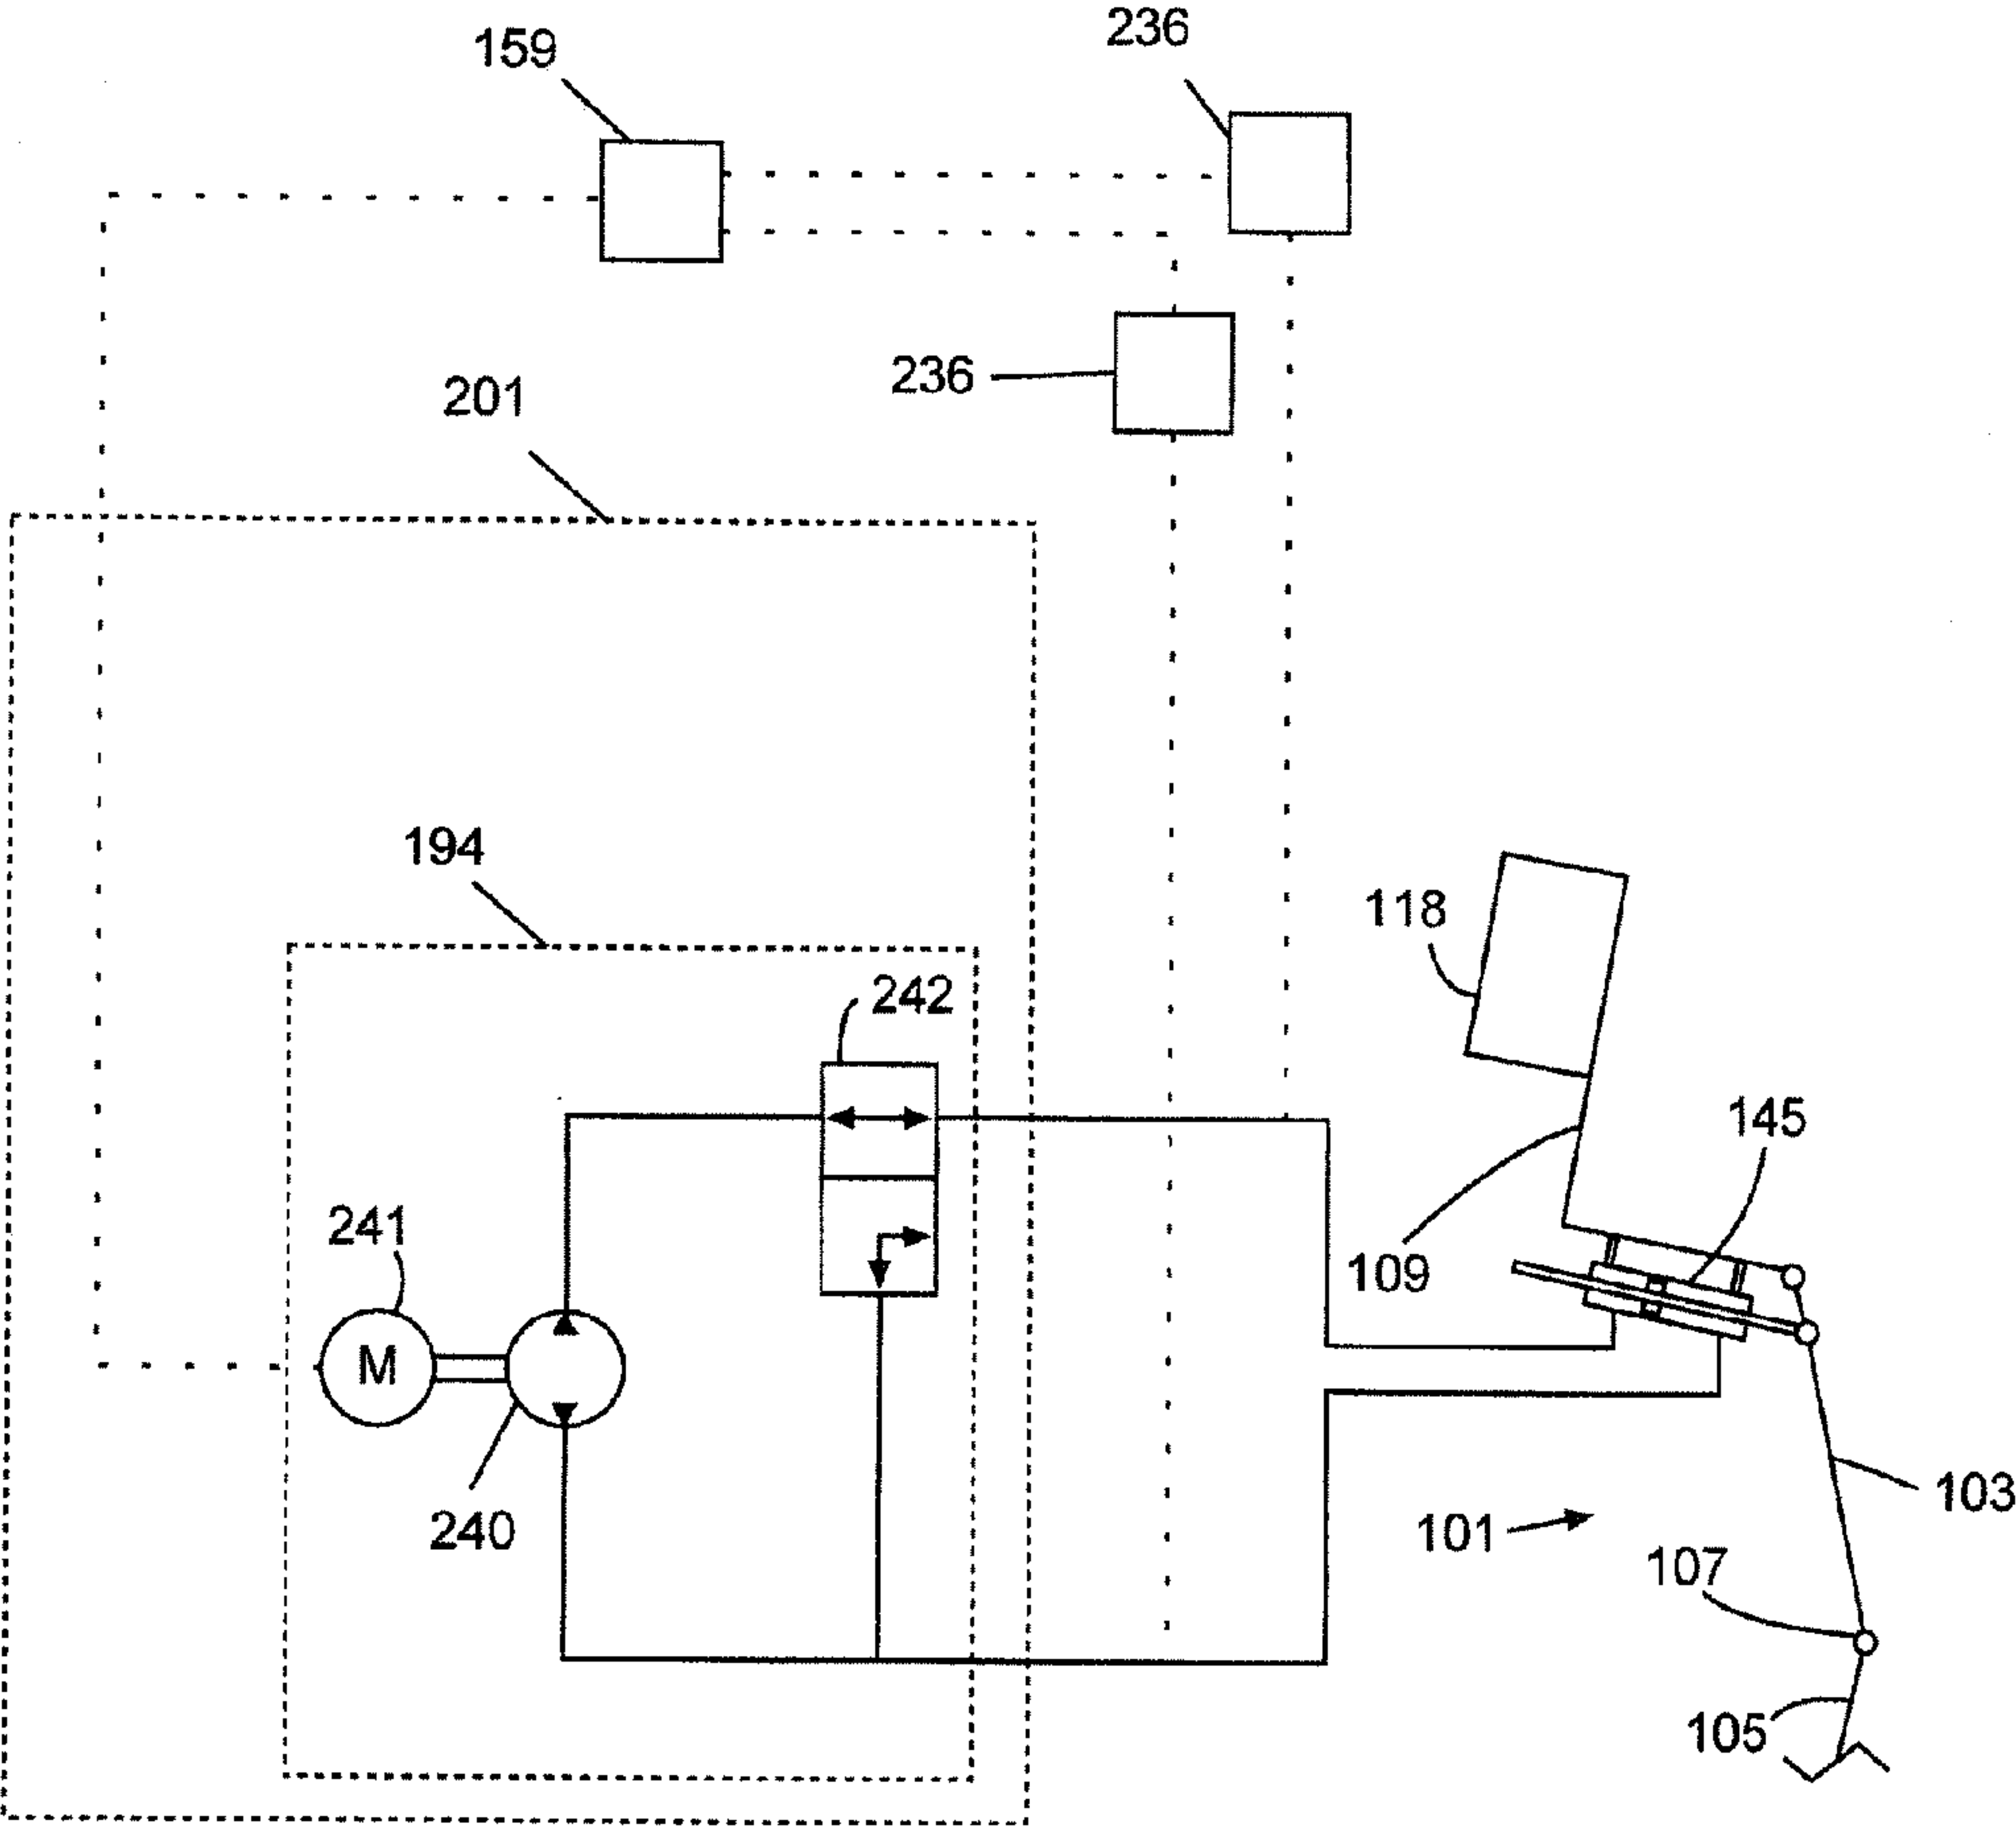


Figure 8

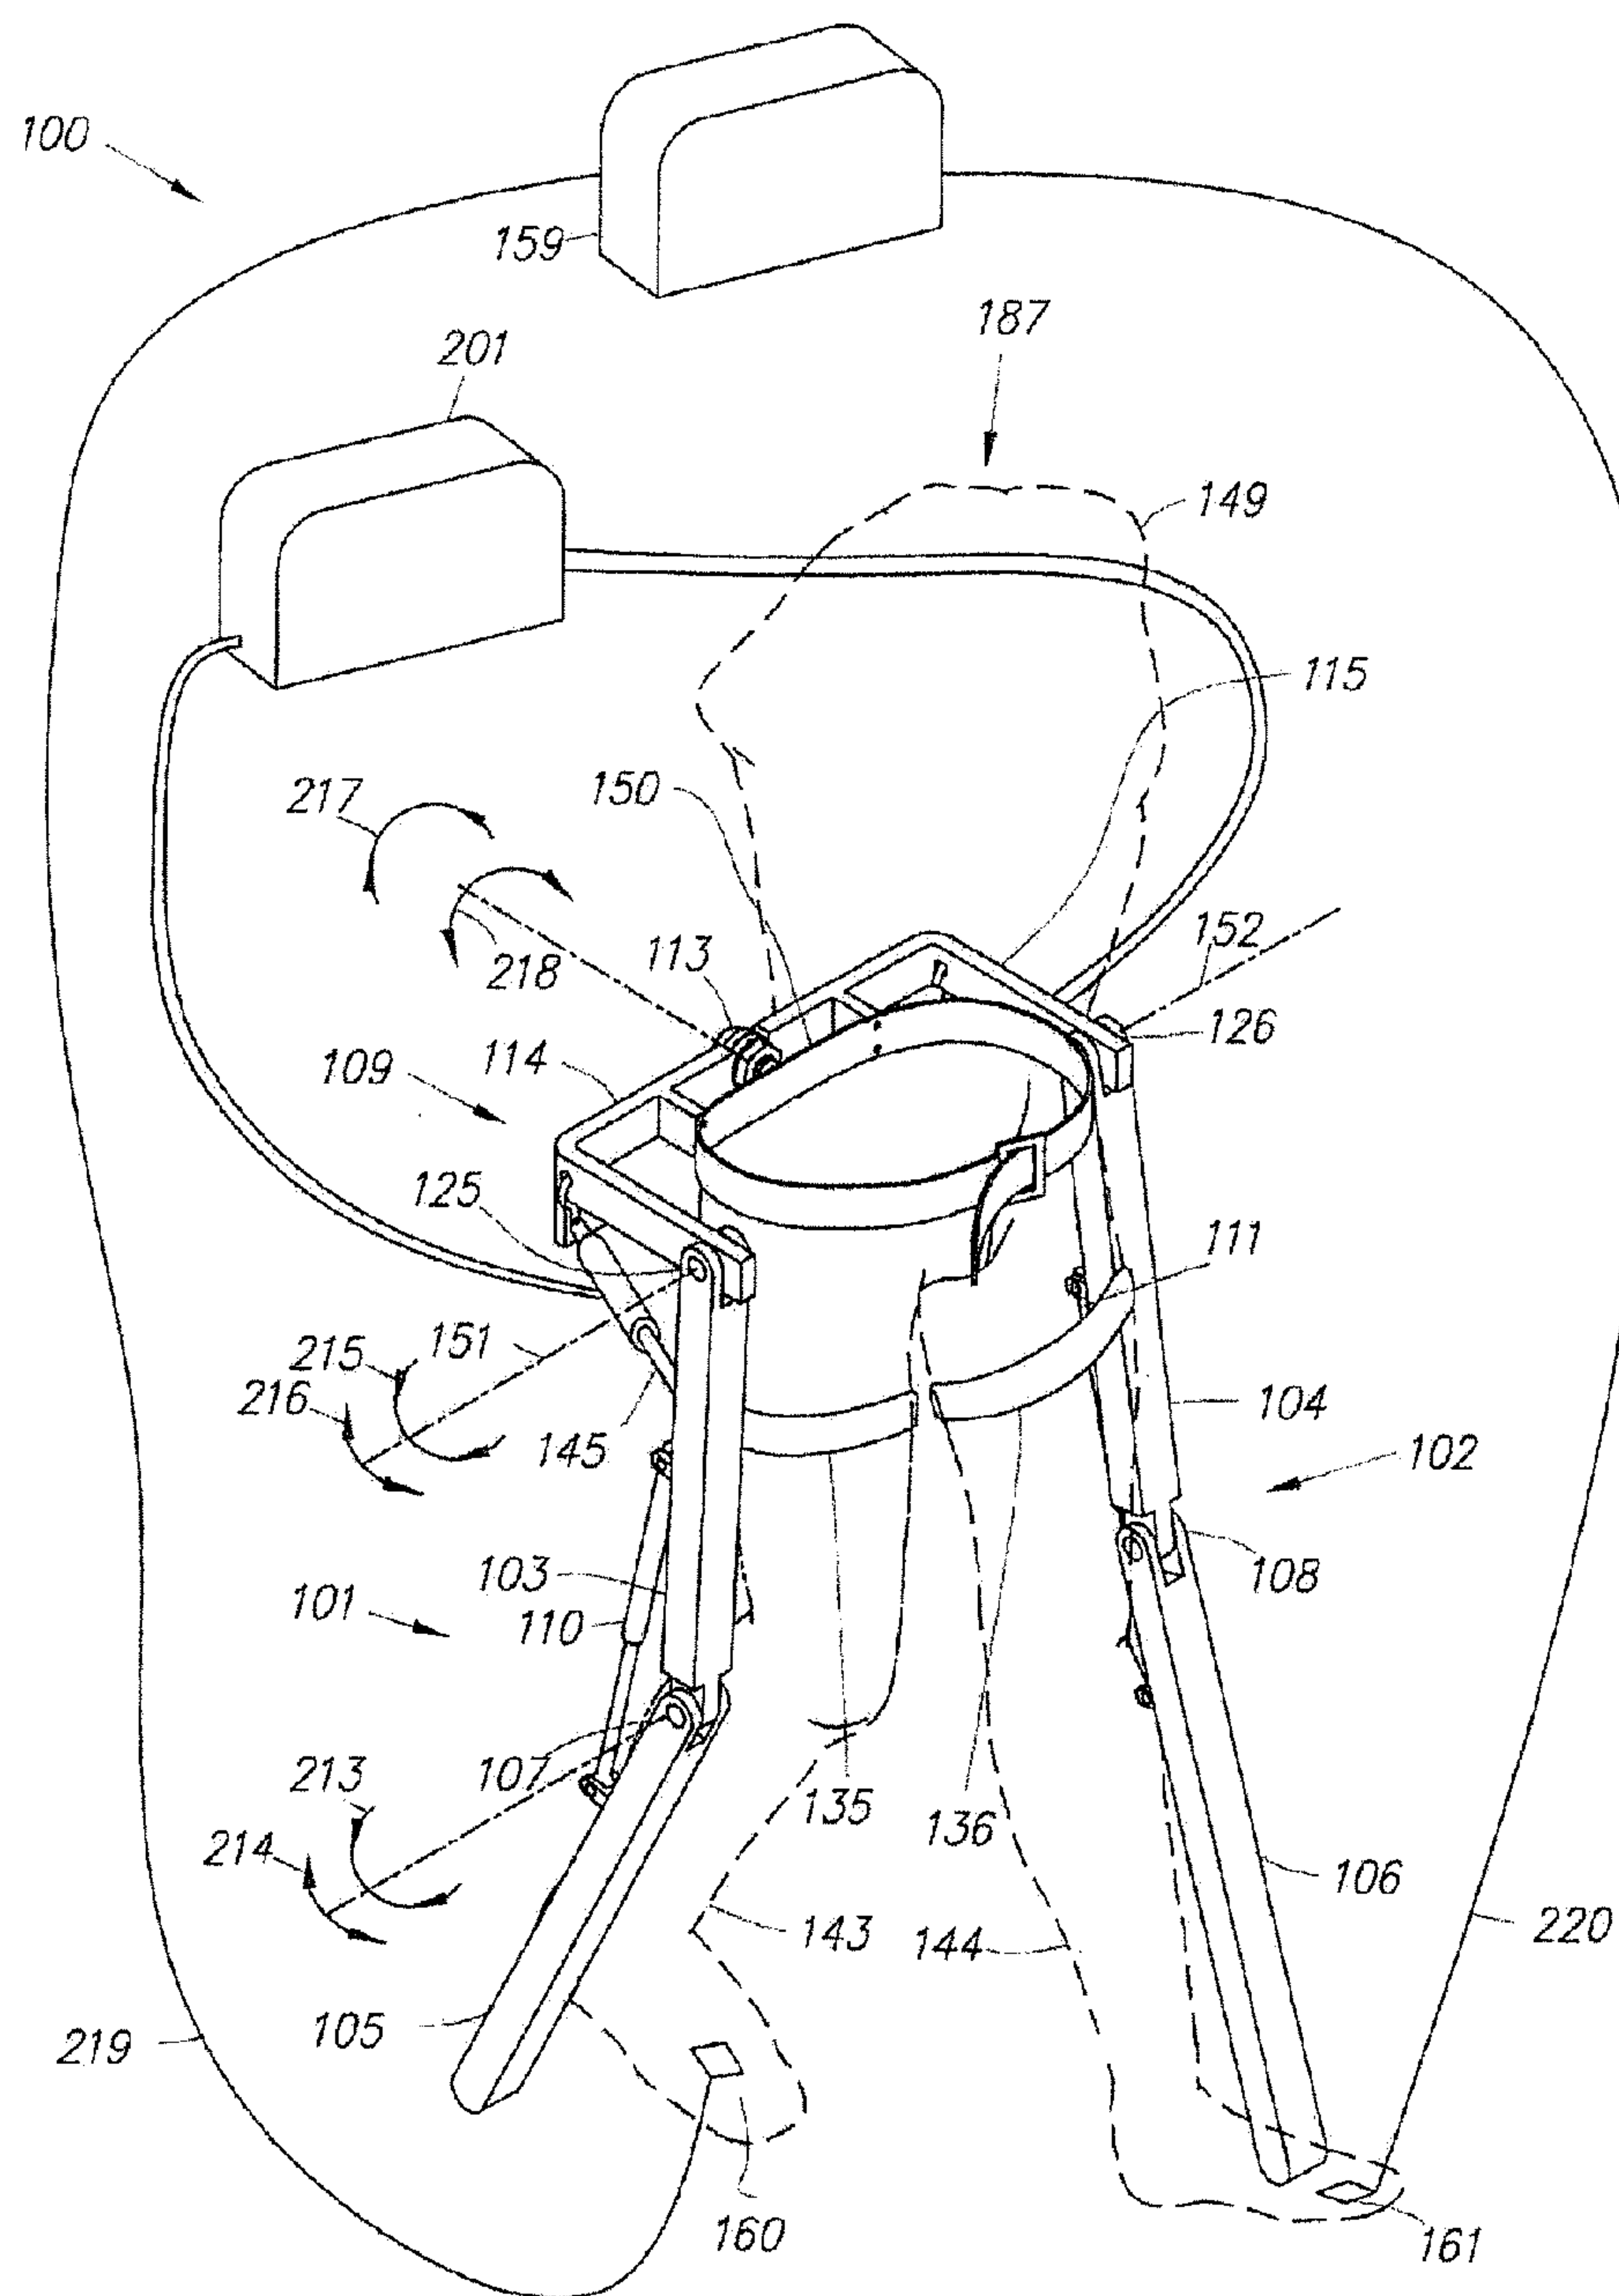
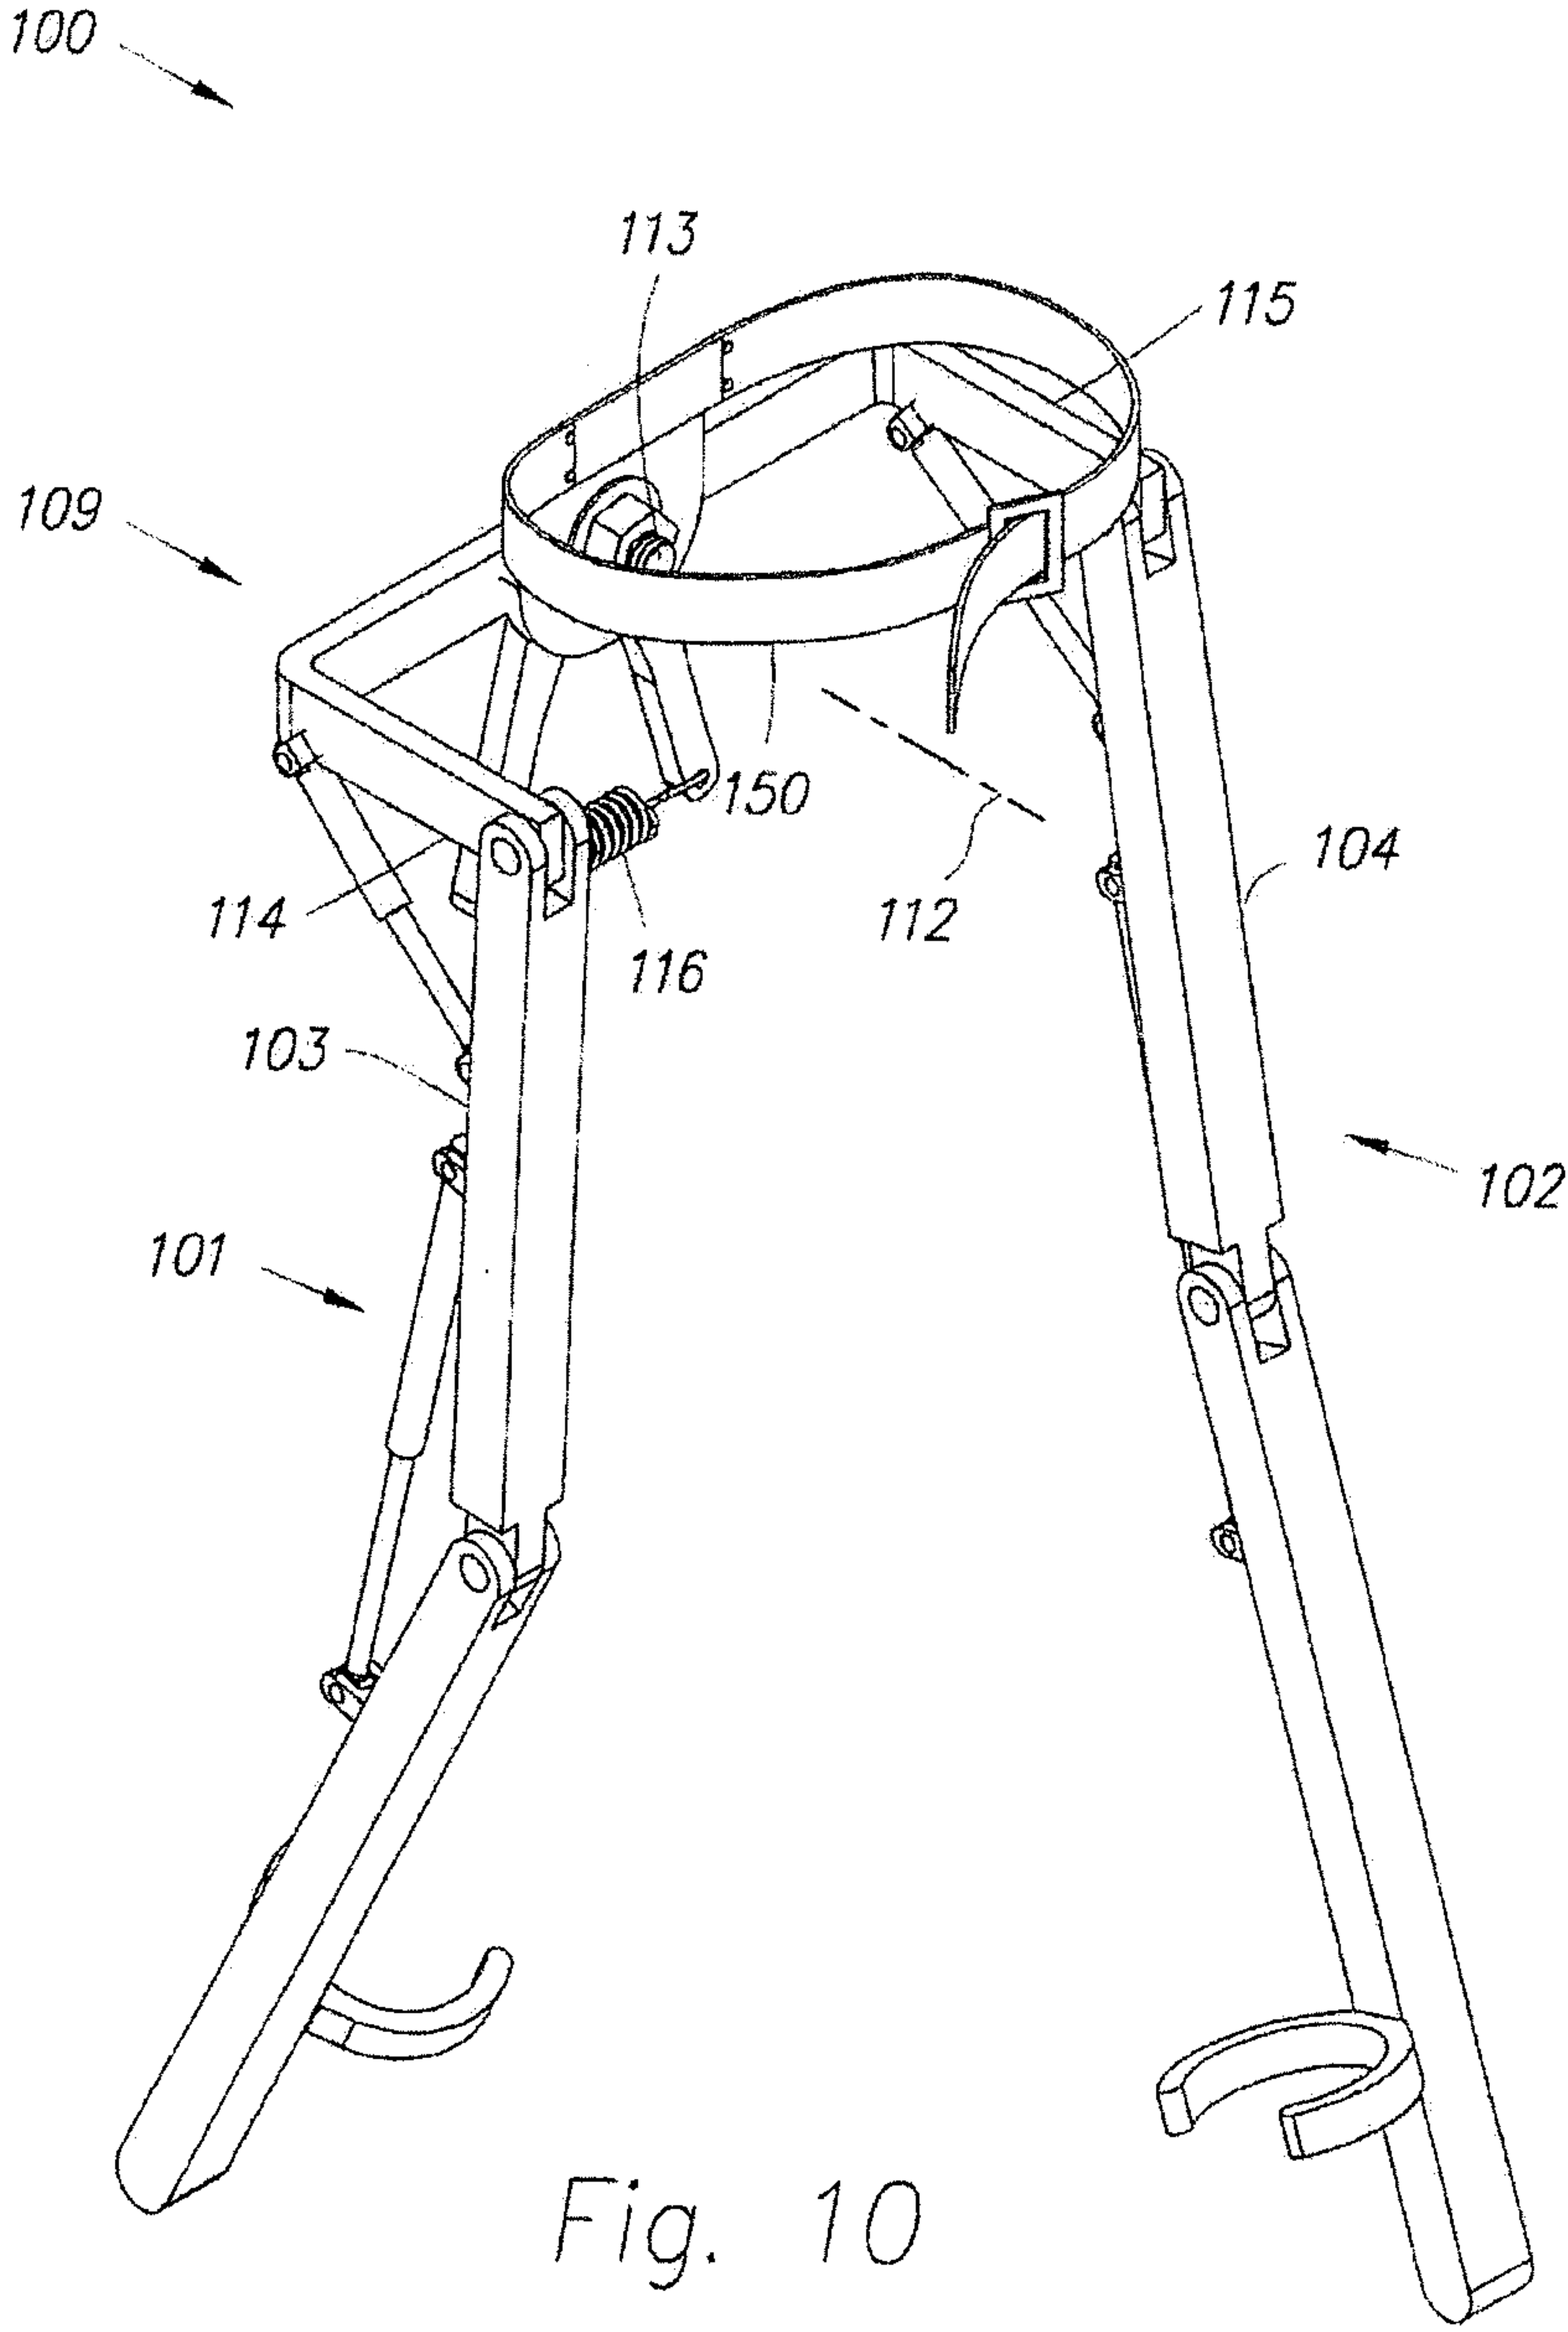
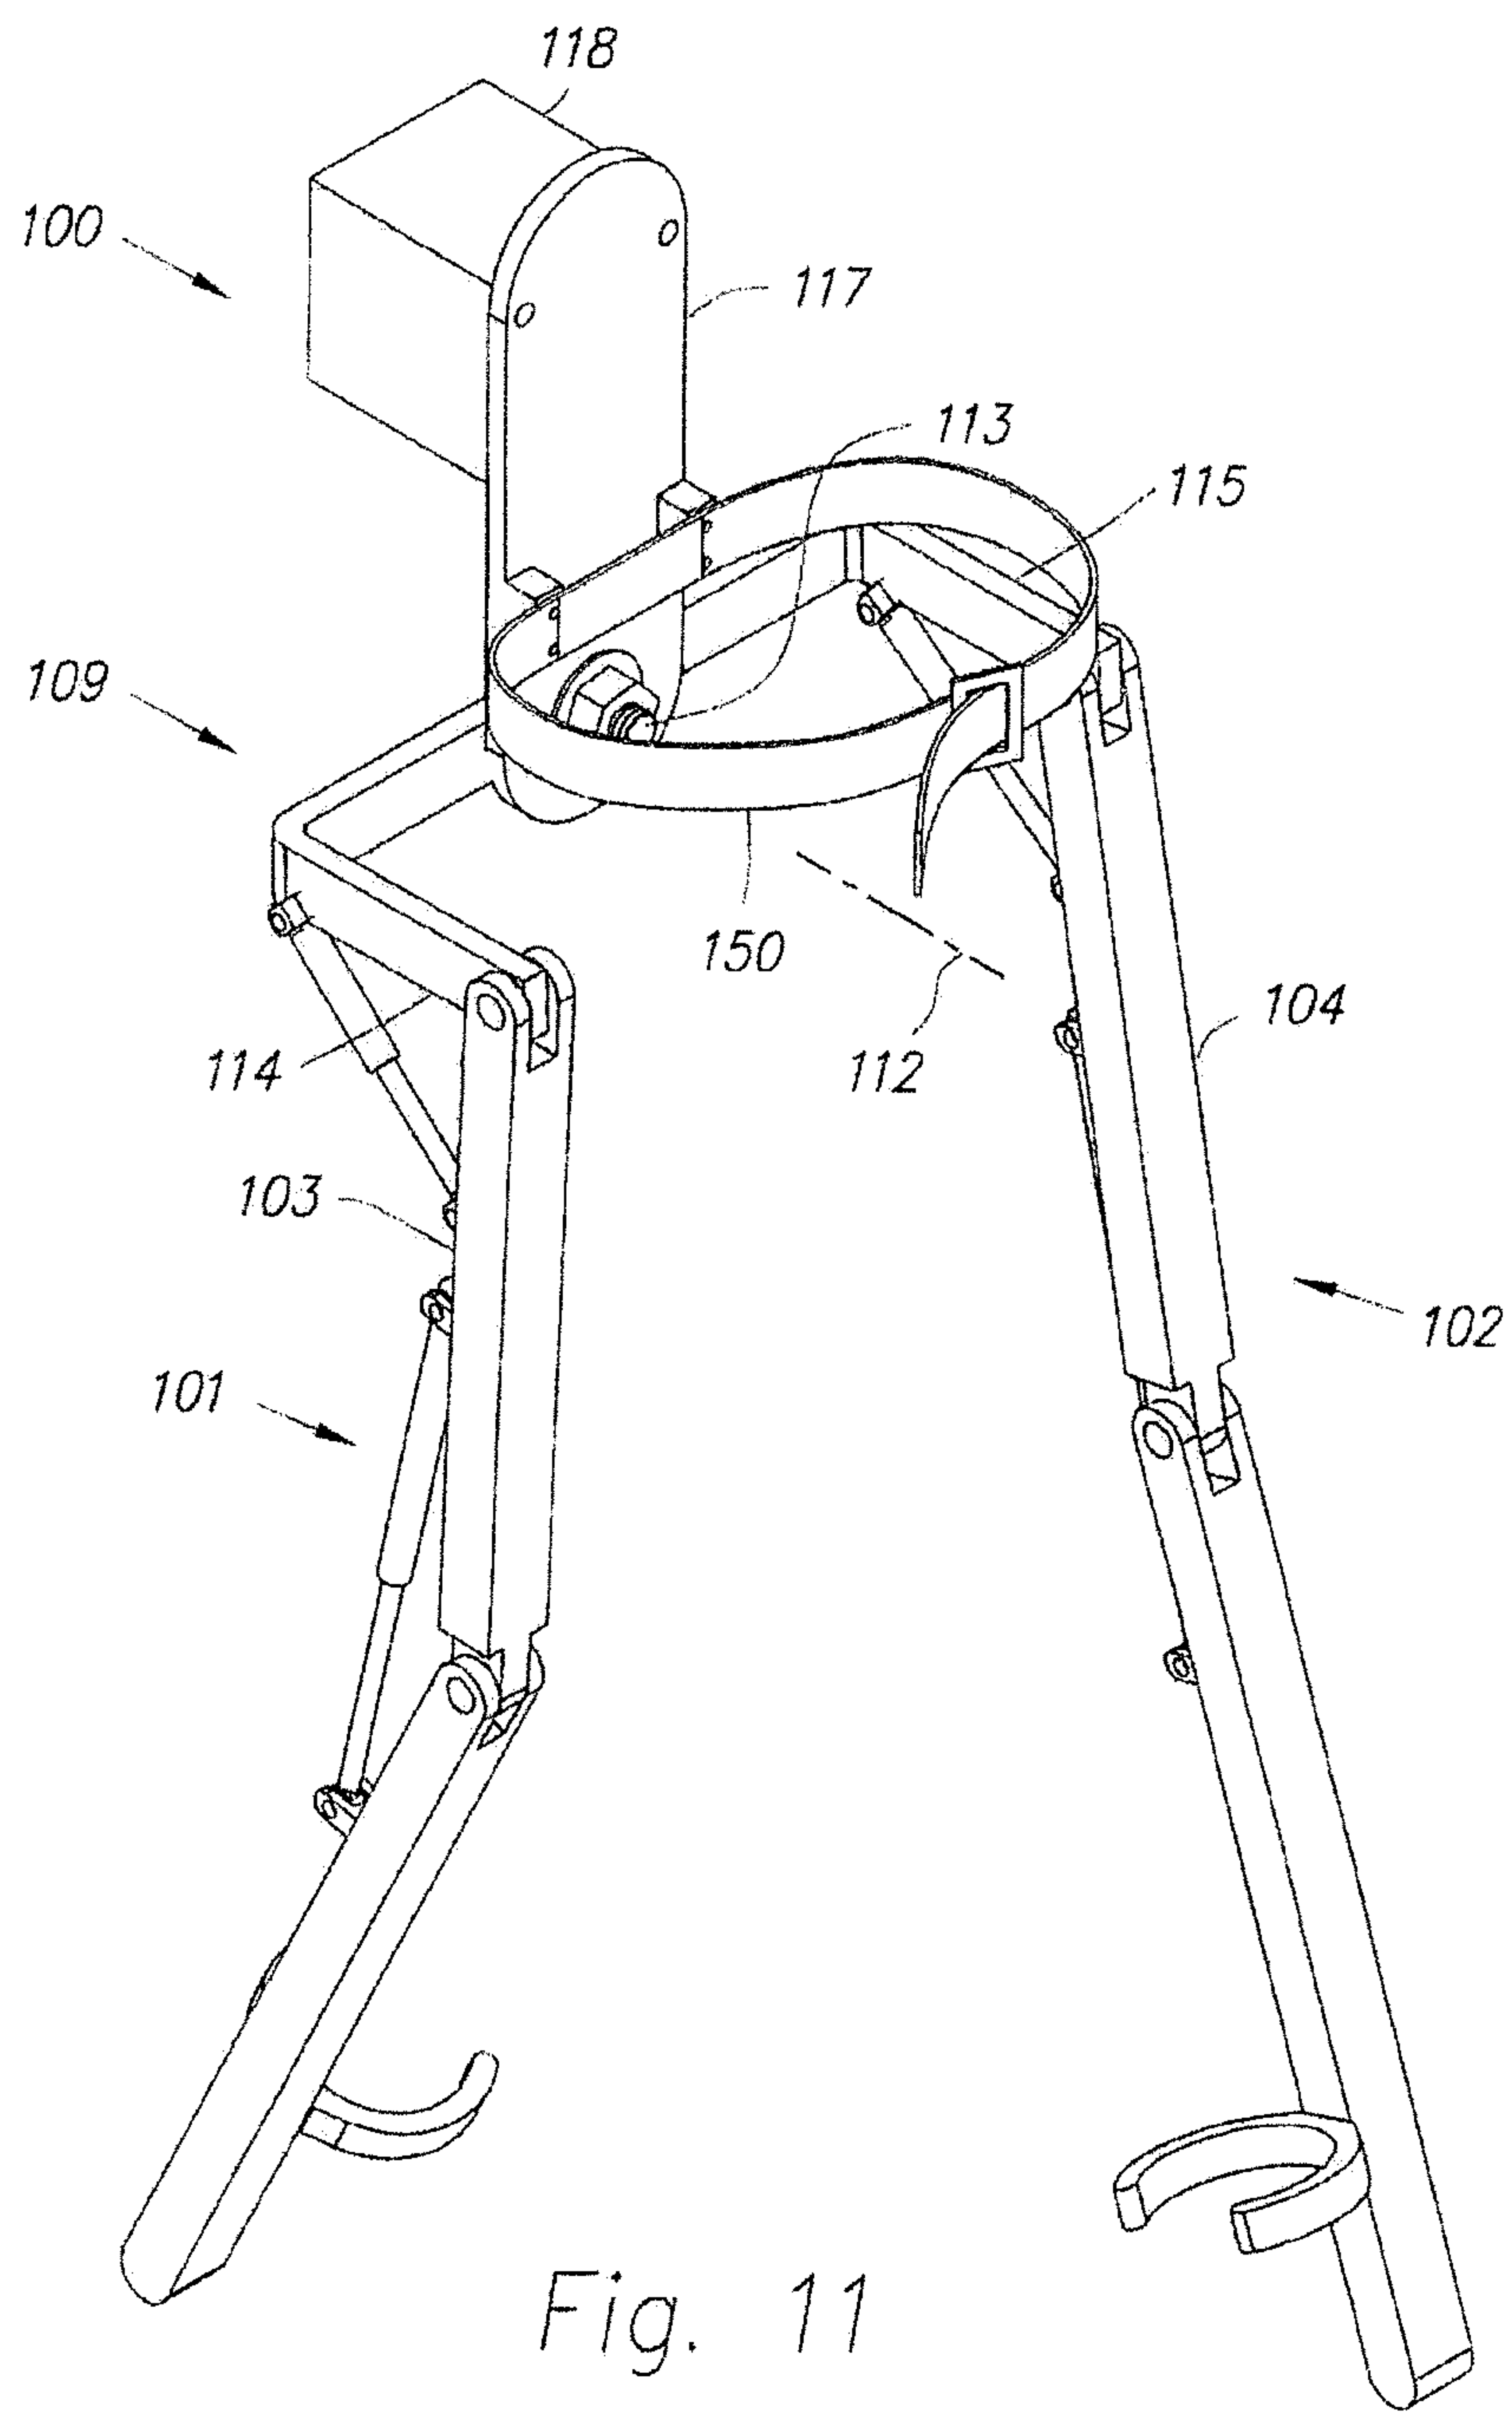
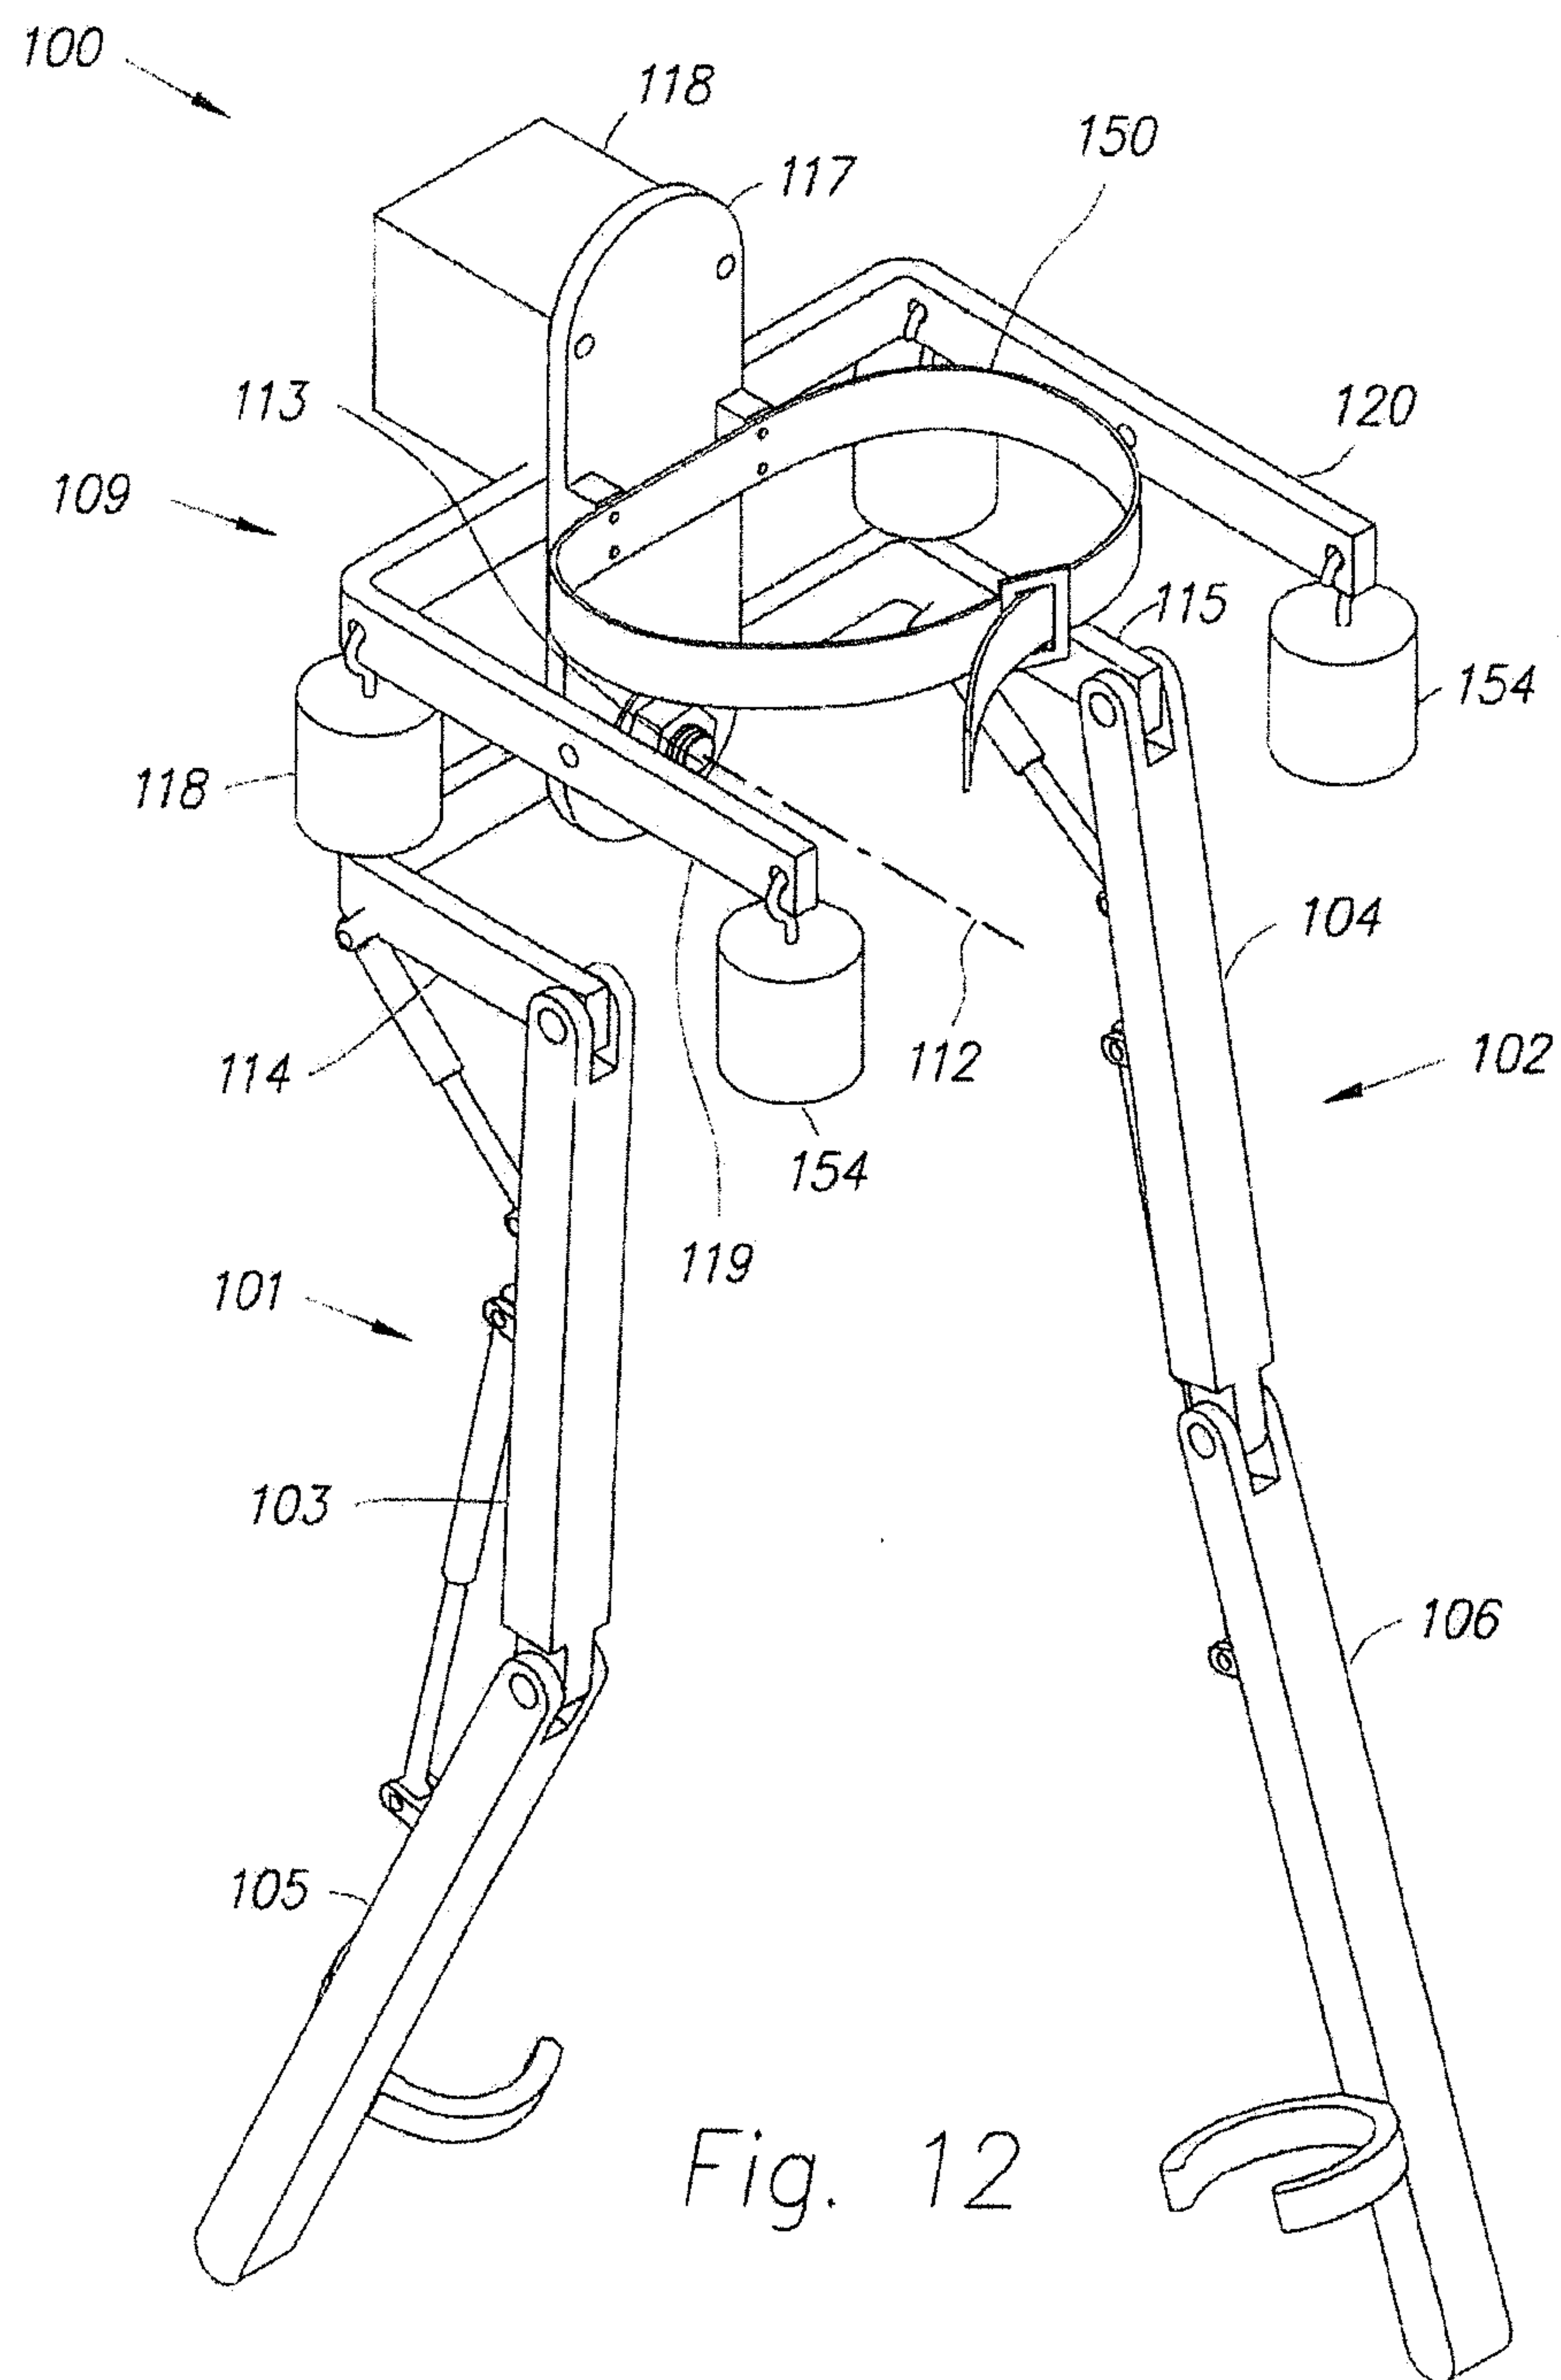


Fig. 9







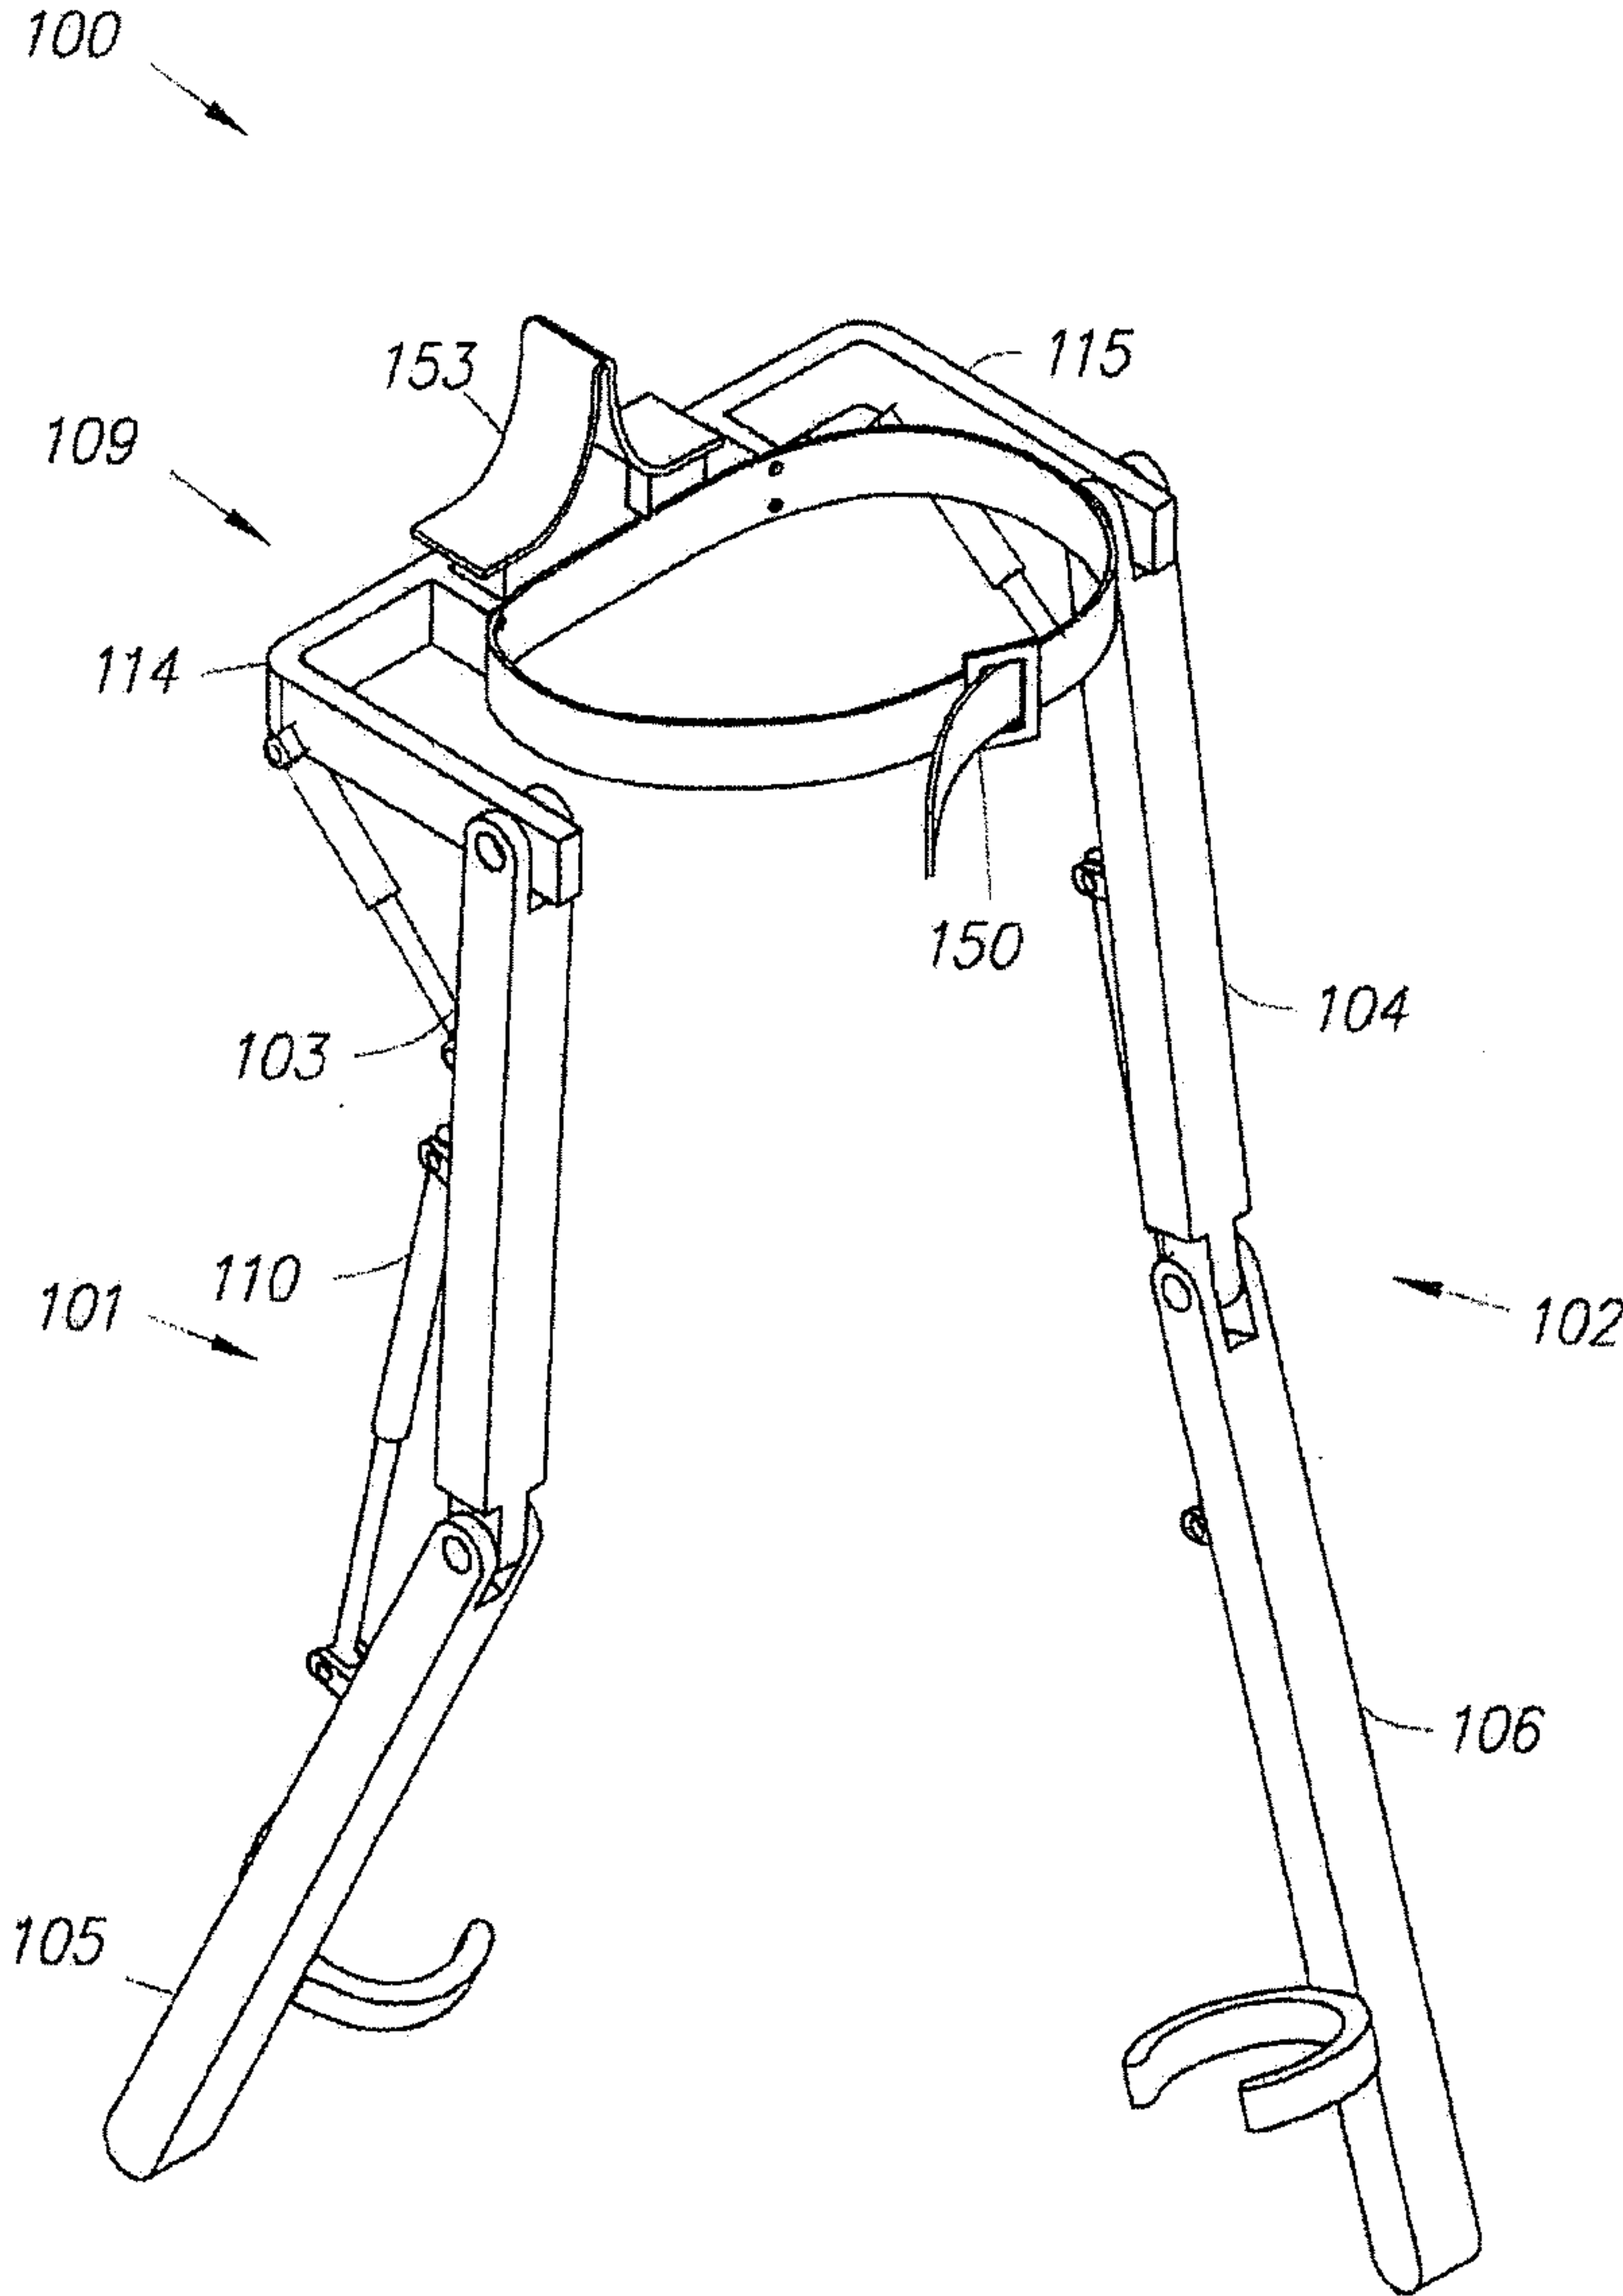
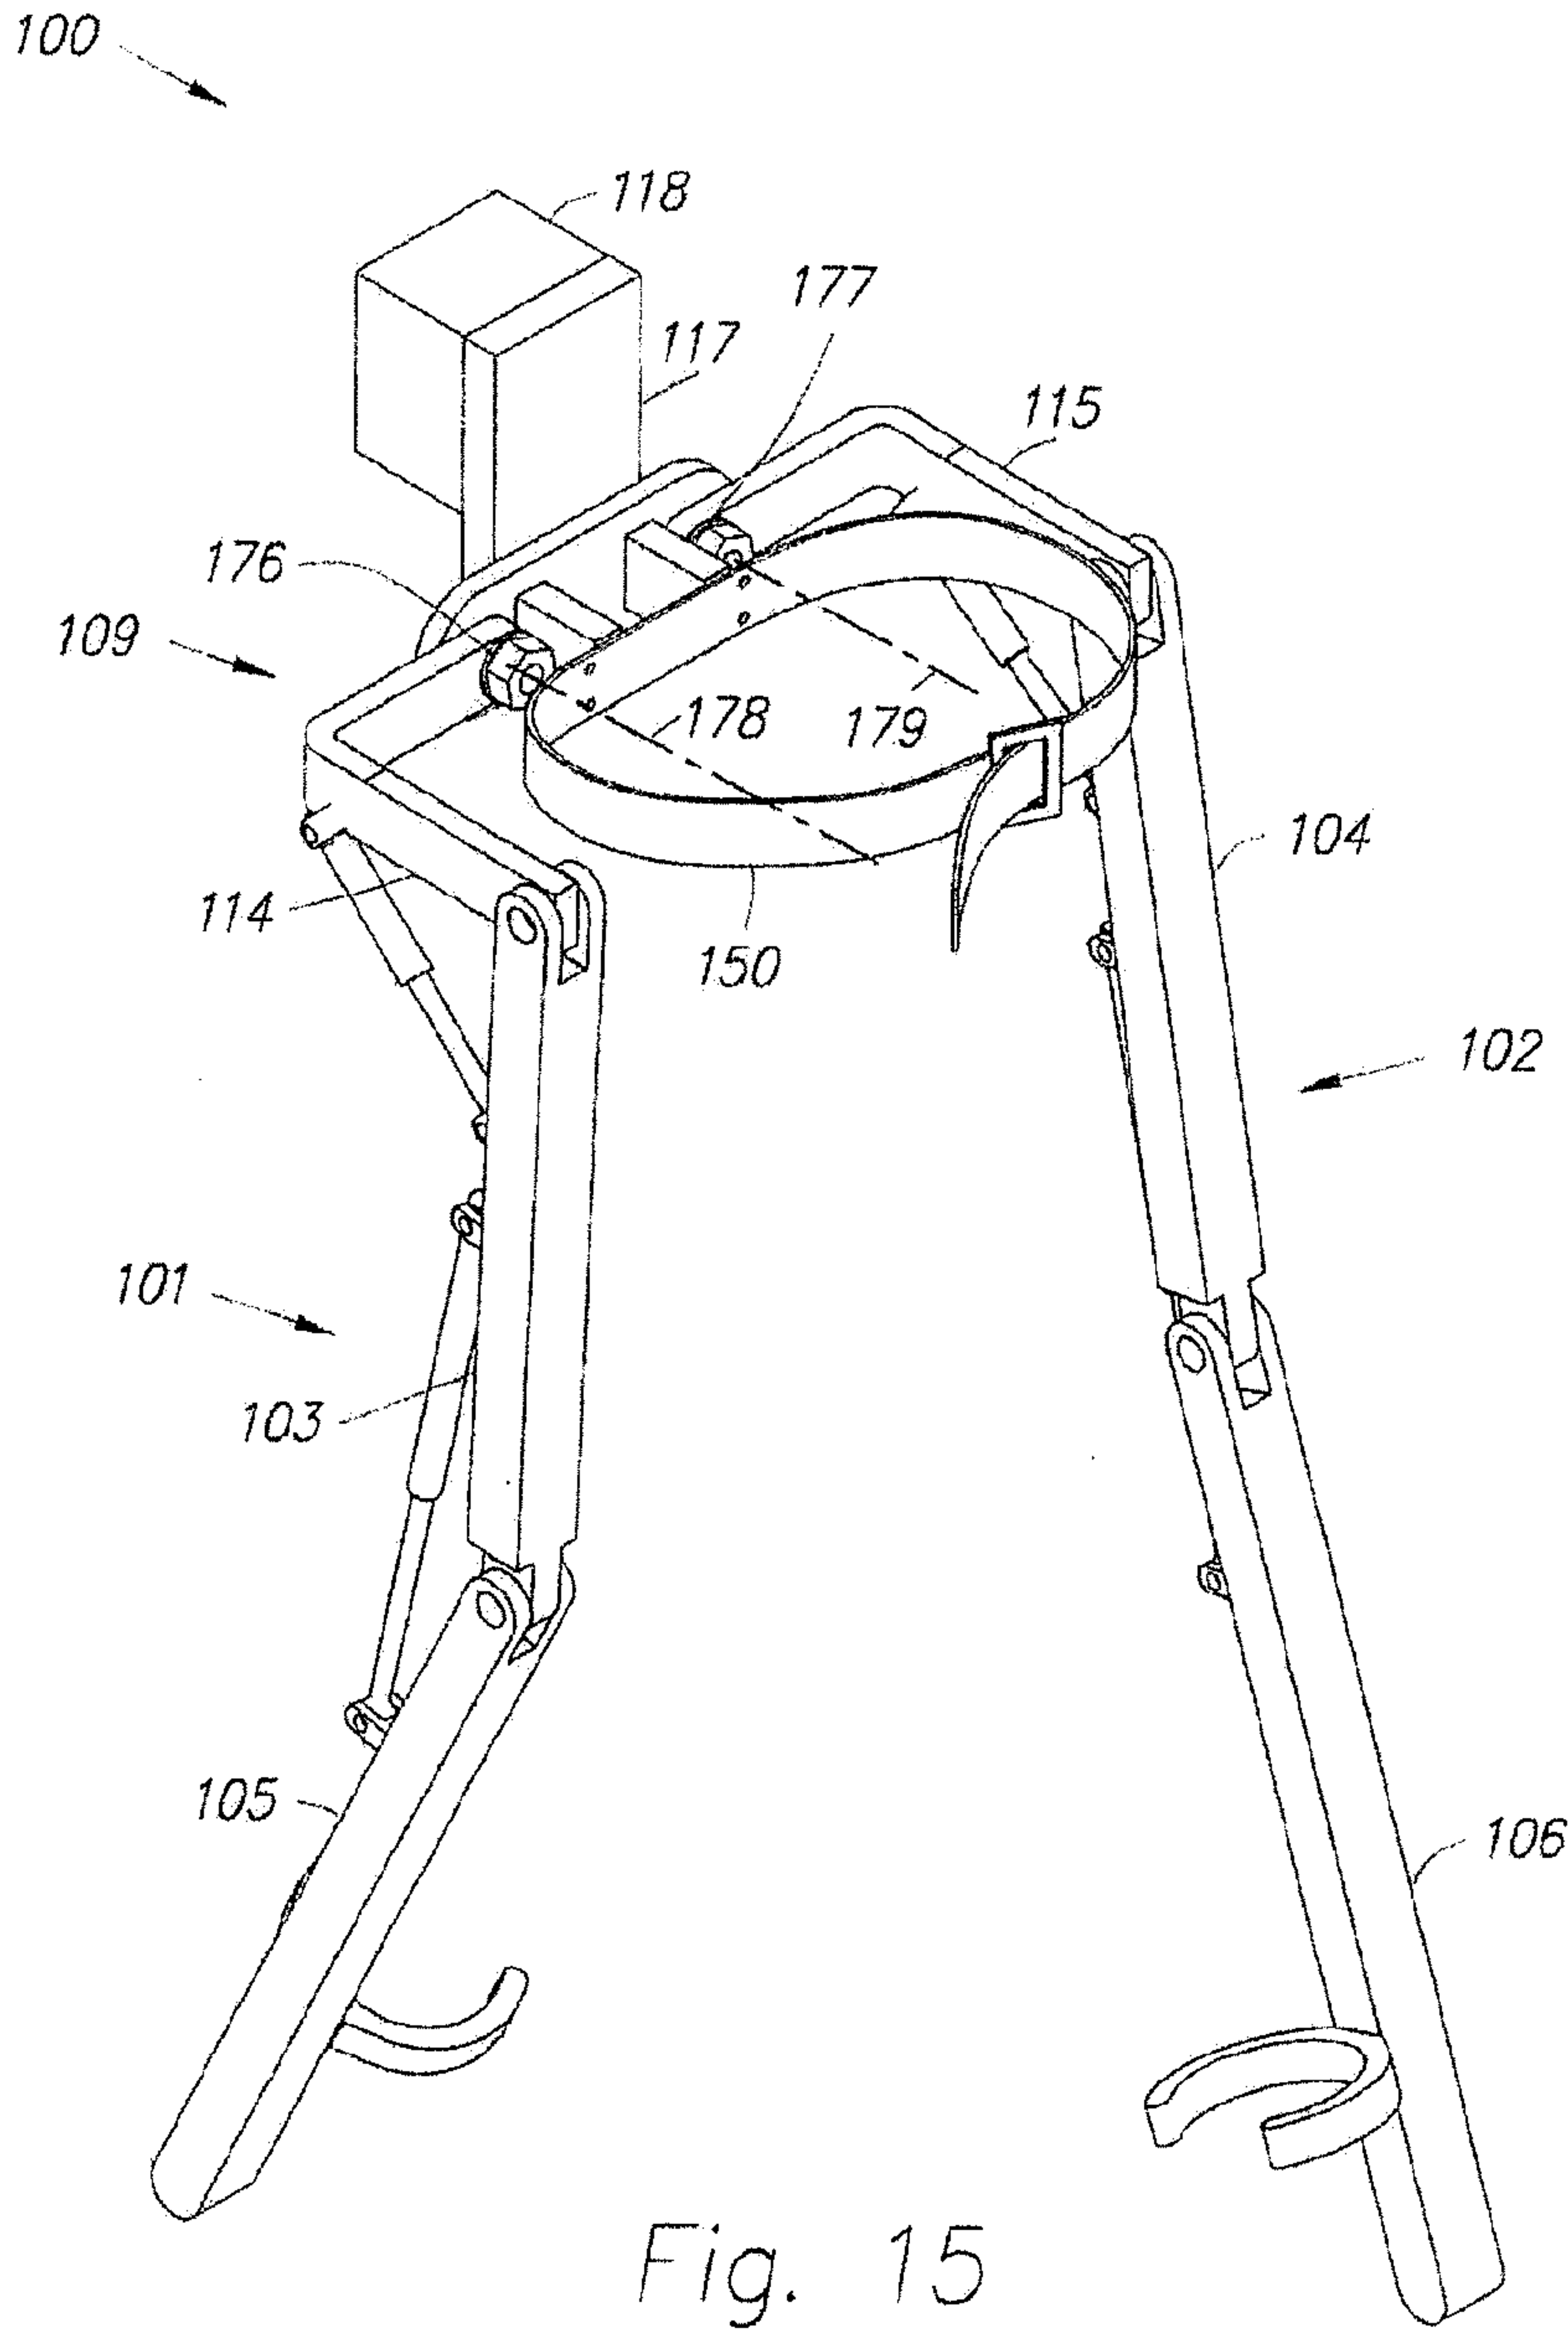


Fig. 14



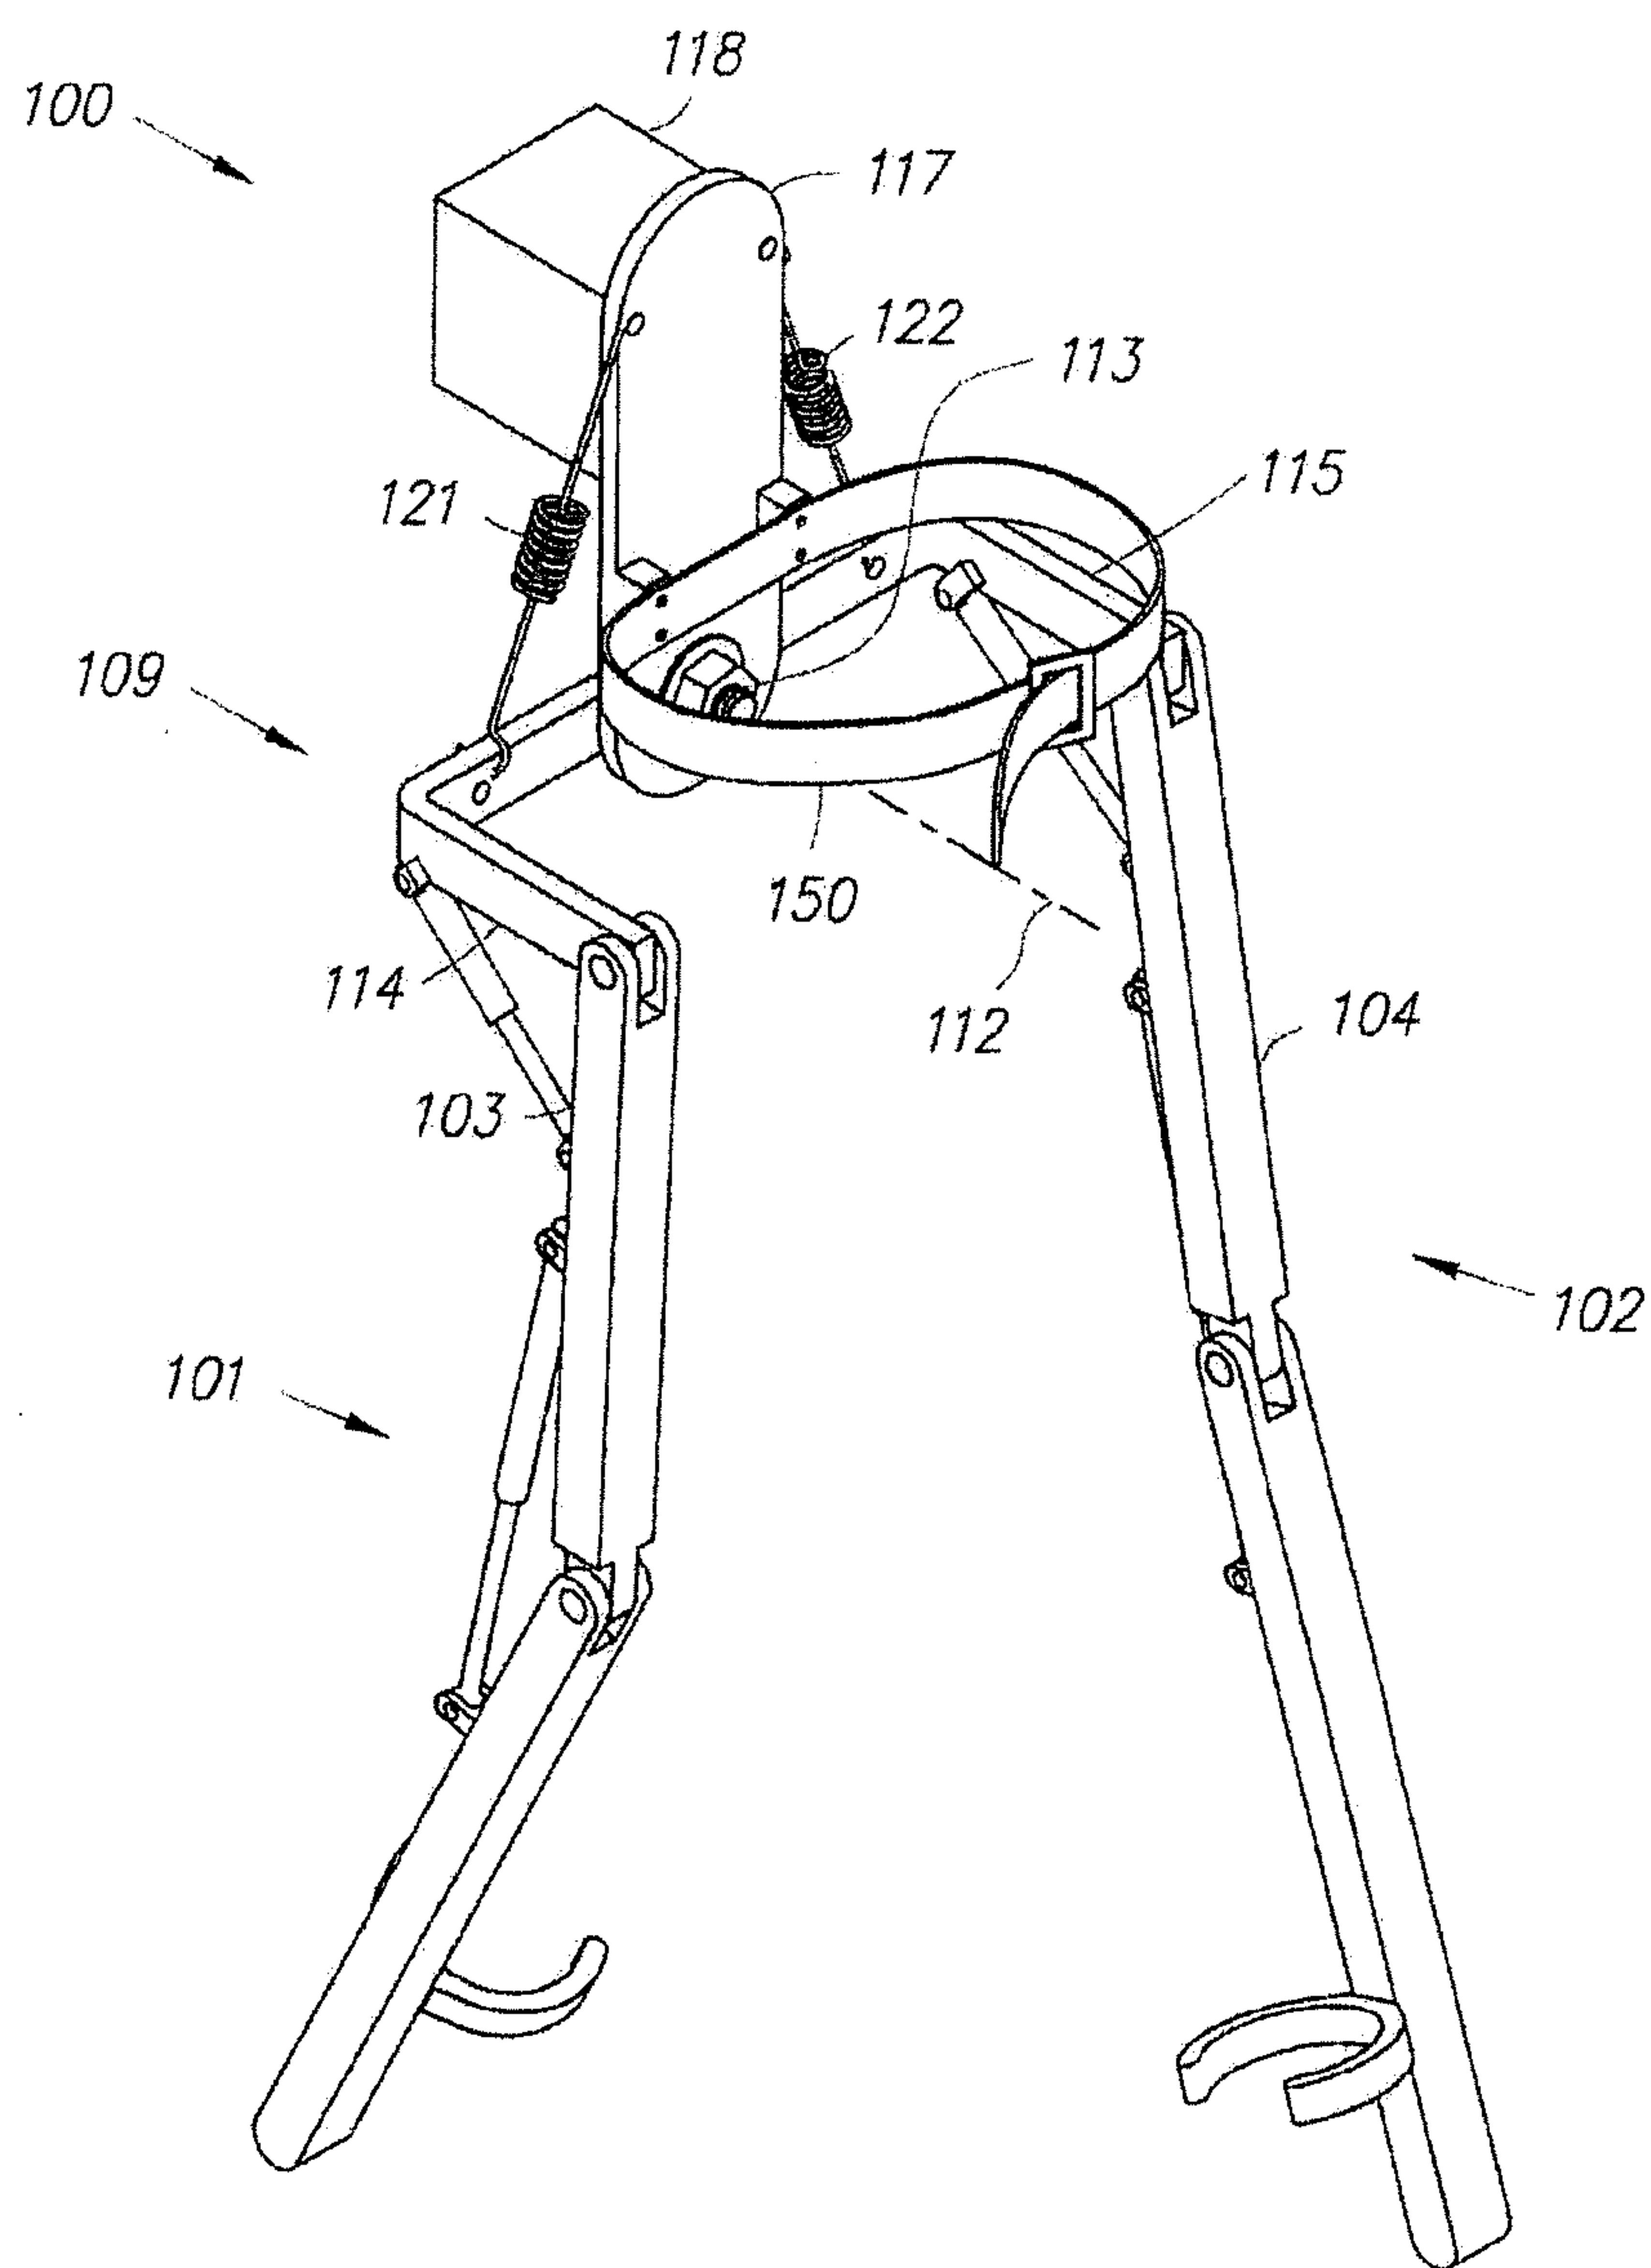


Fig. 16

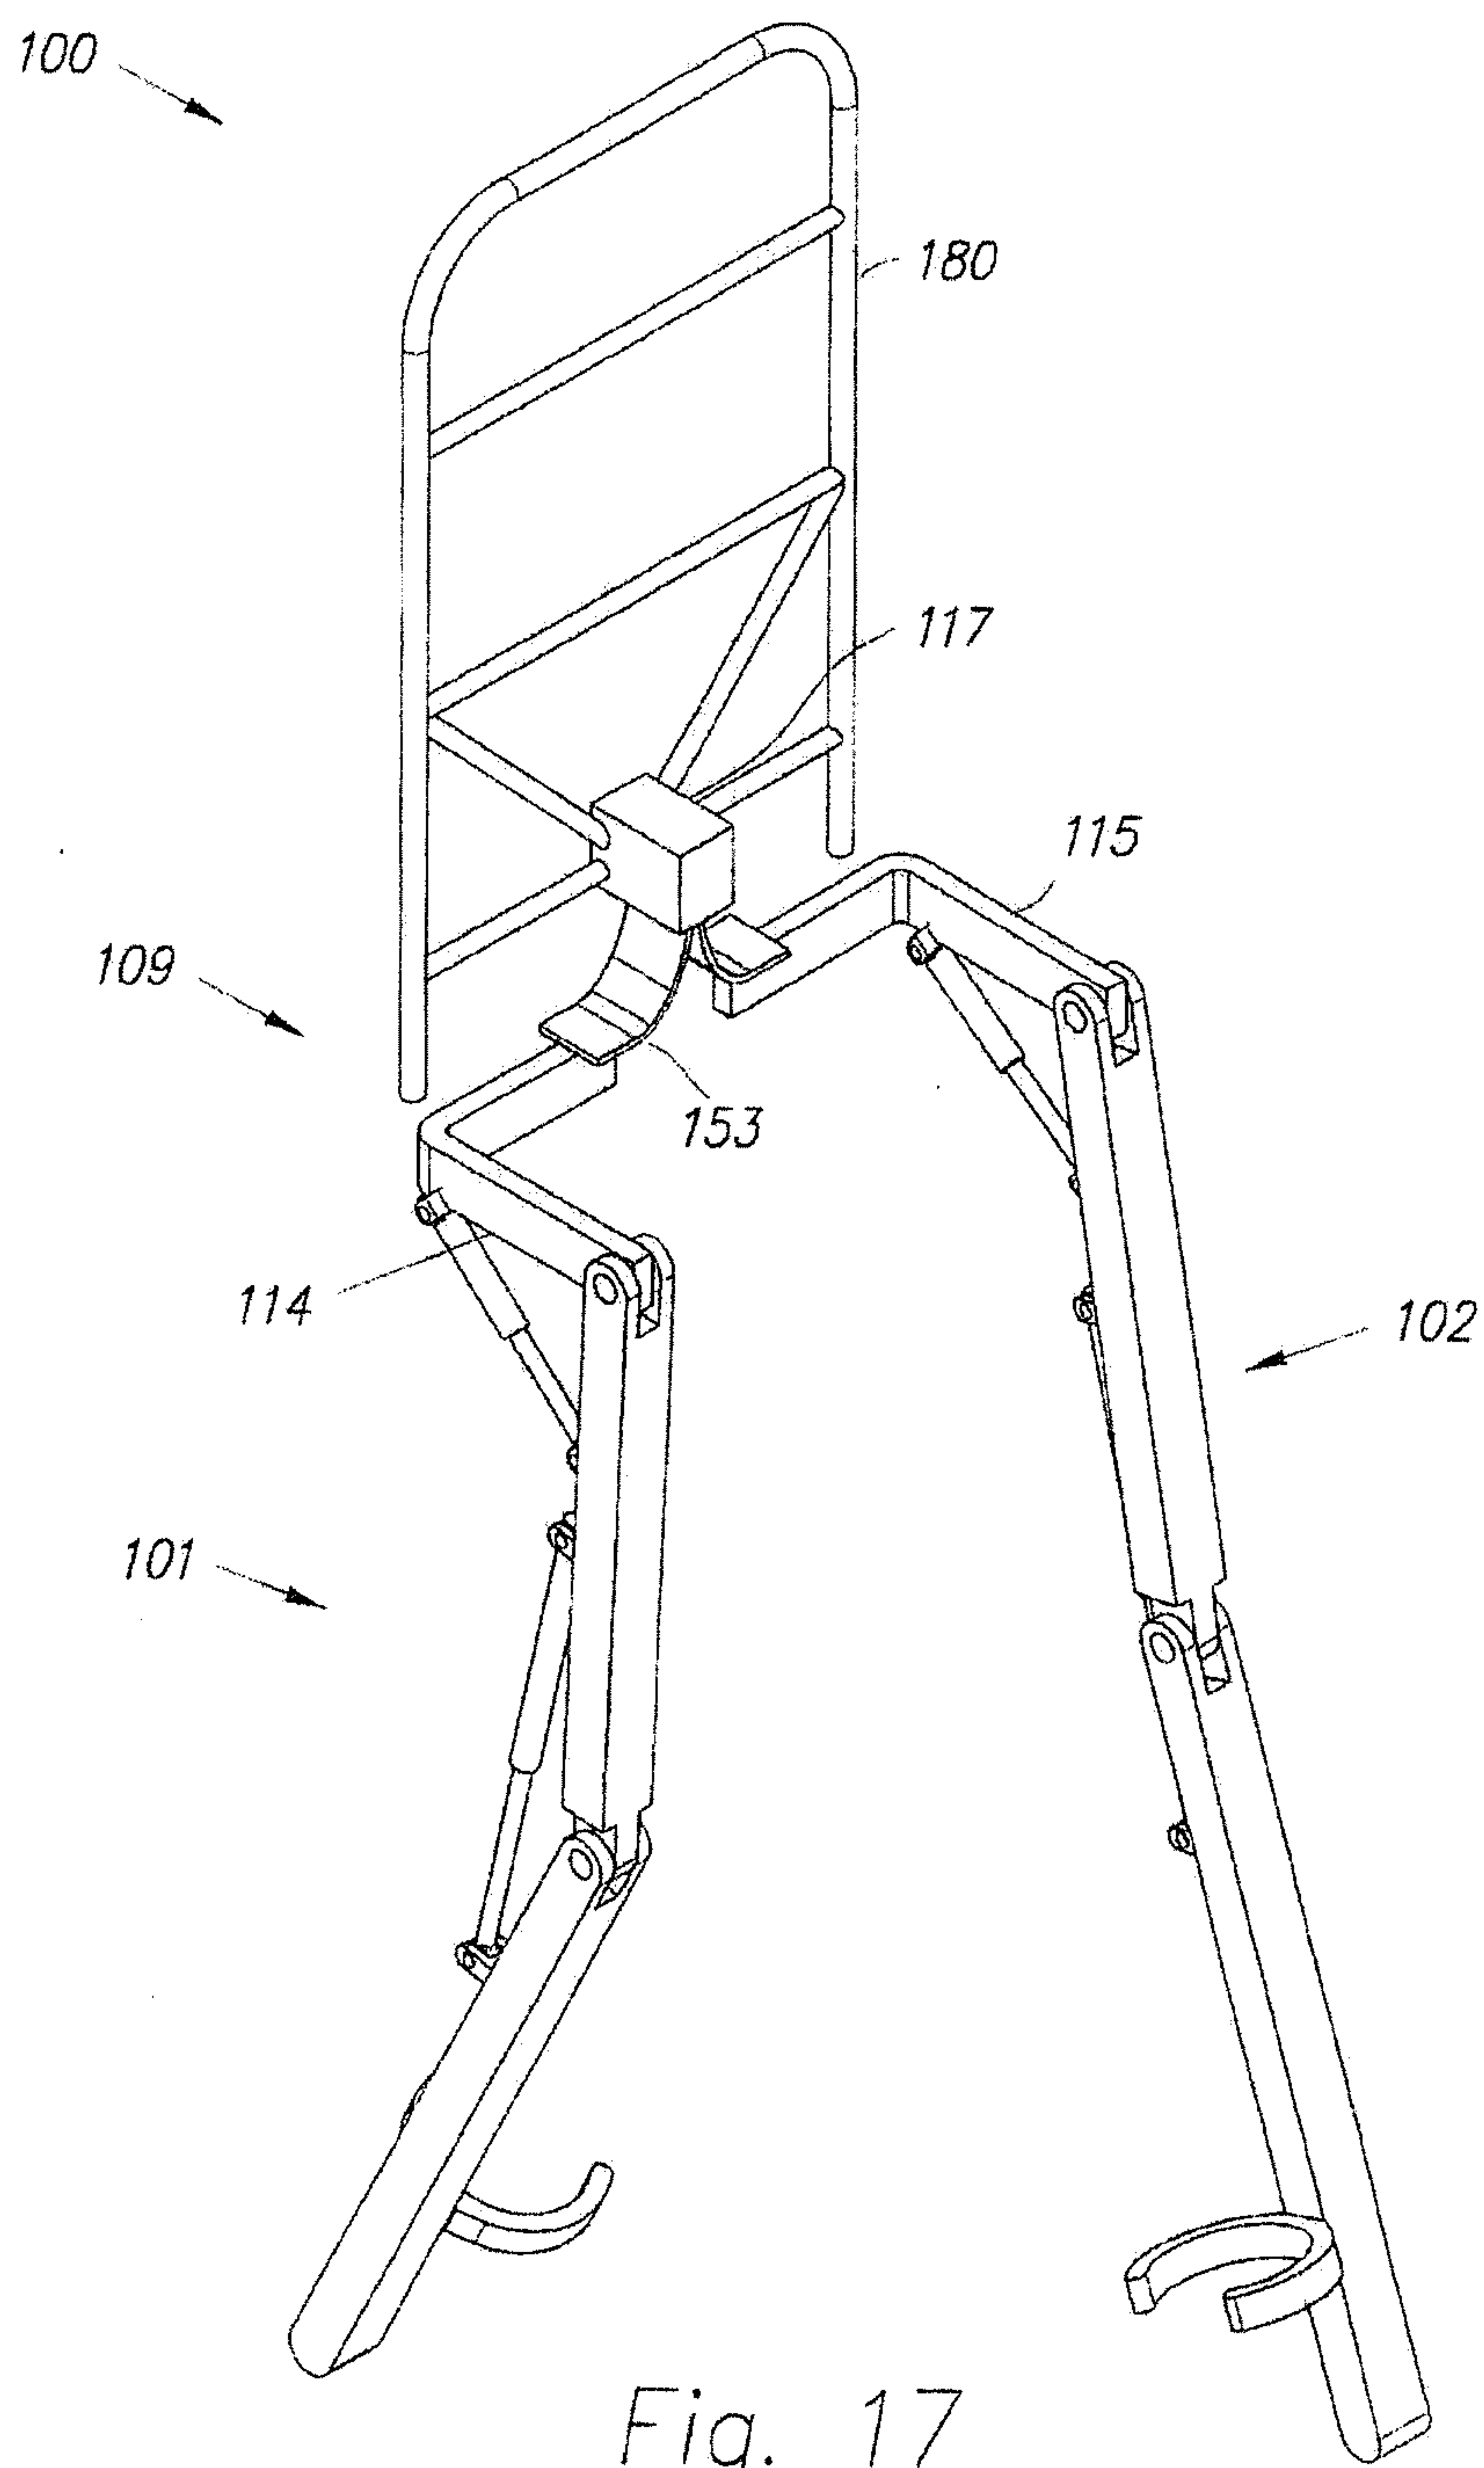


Fig. 17

Fig. 18

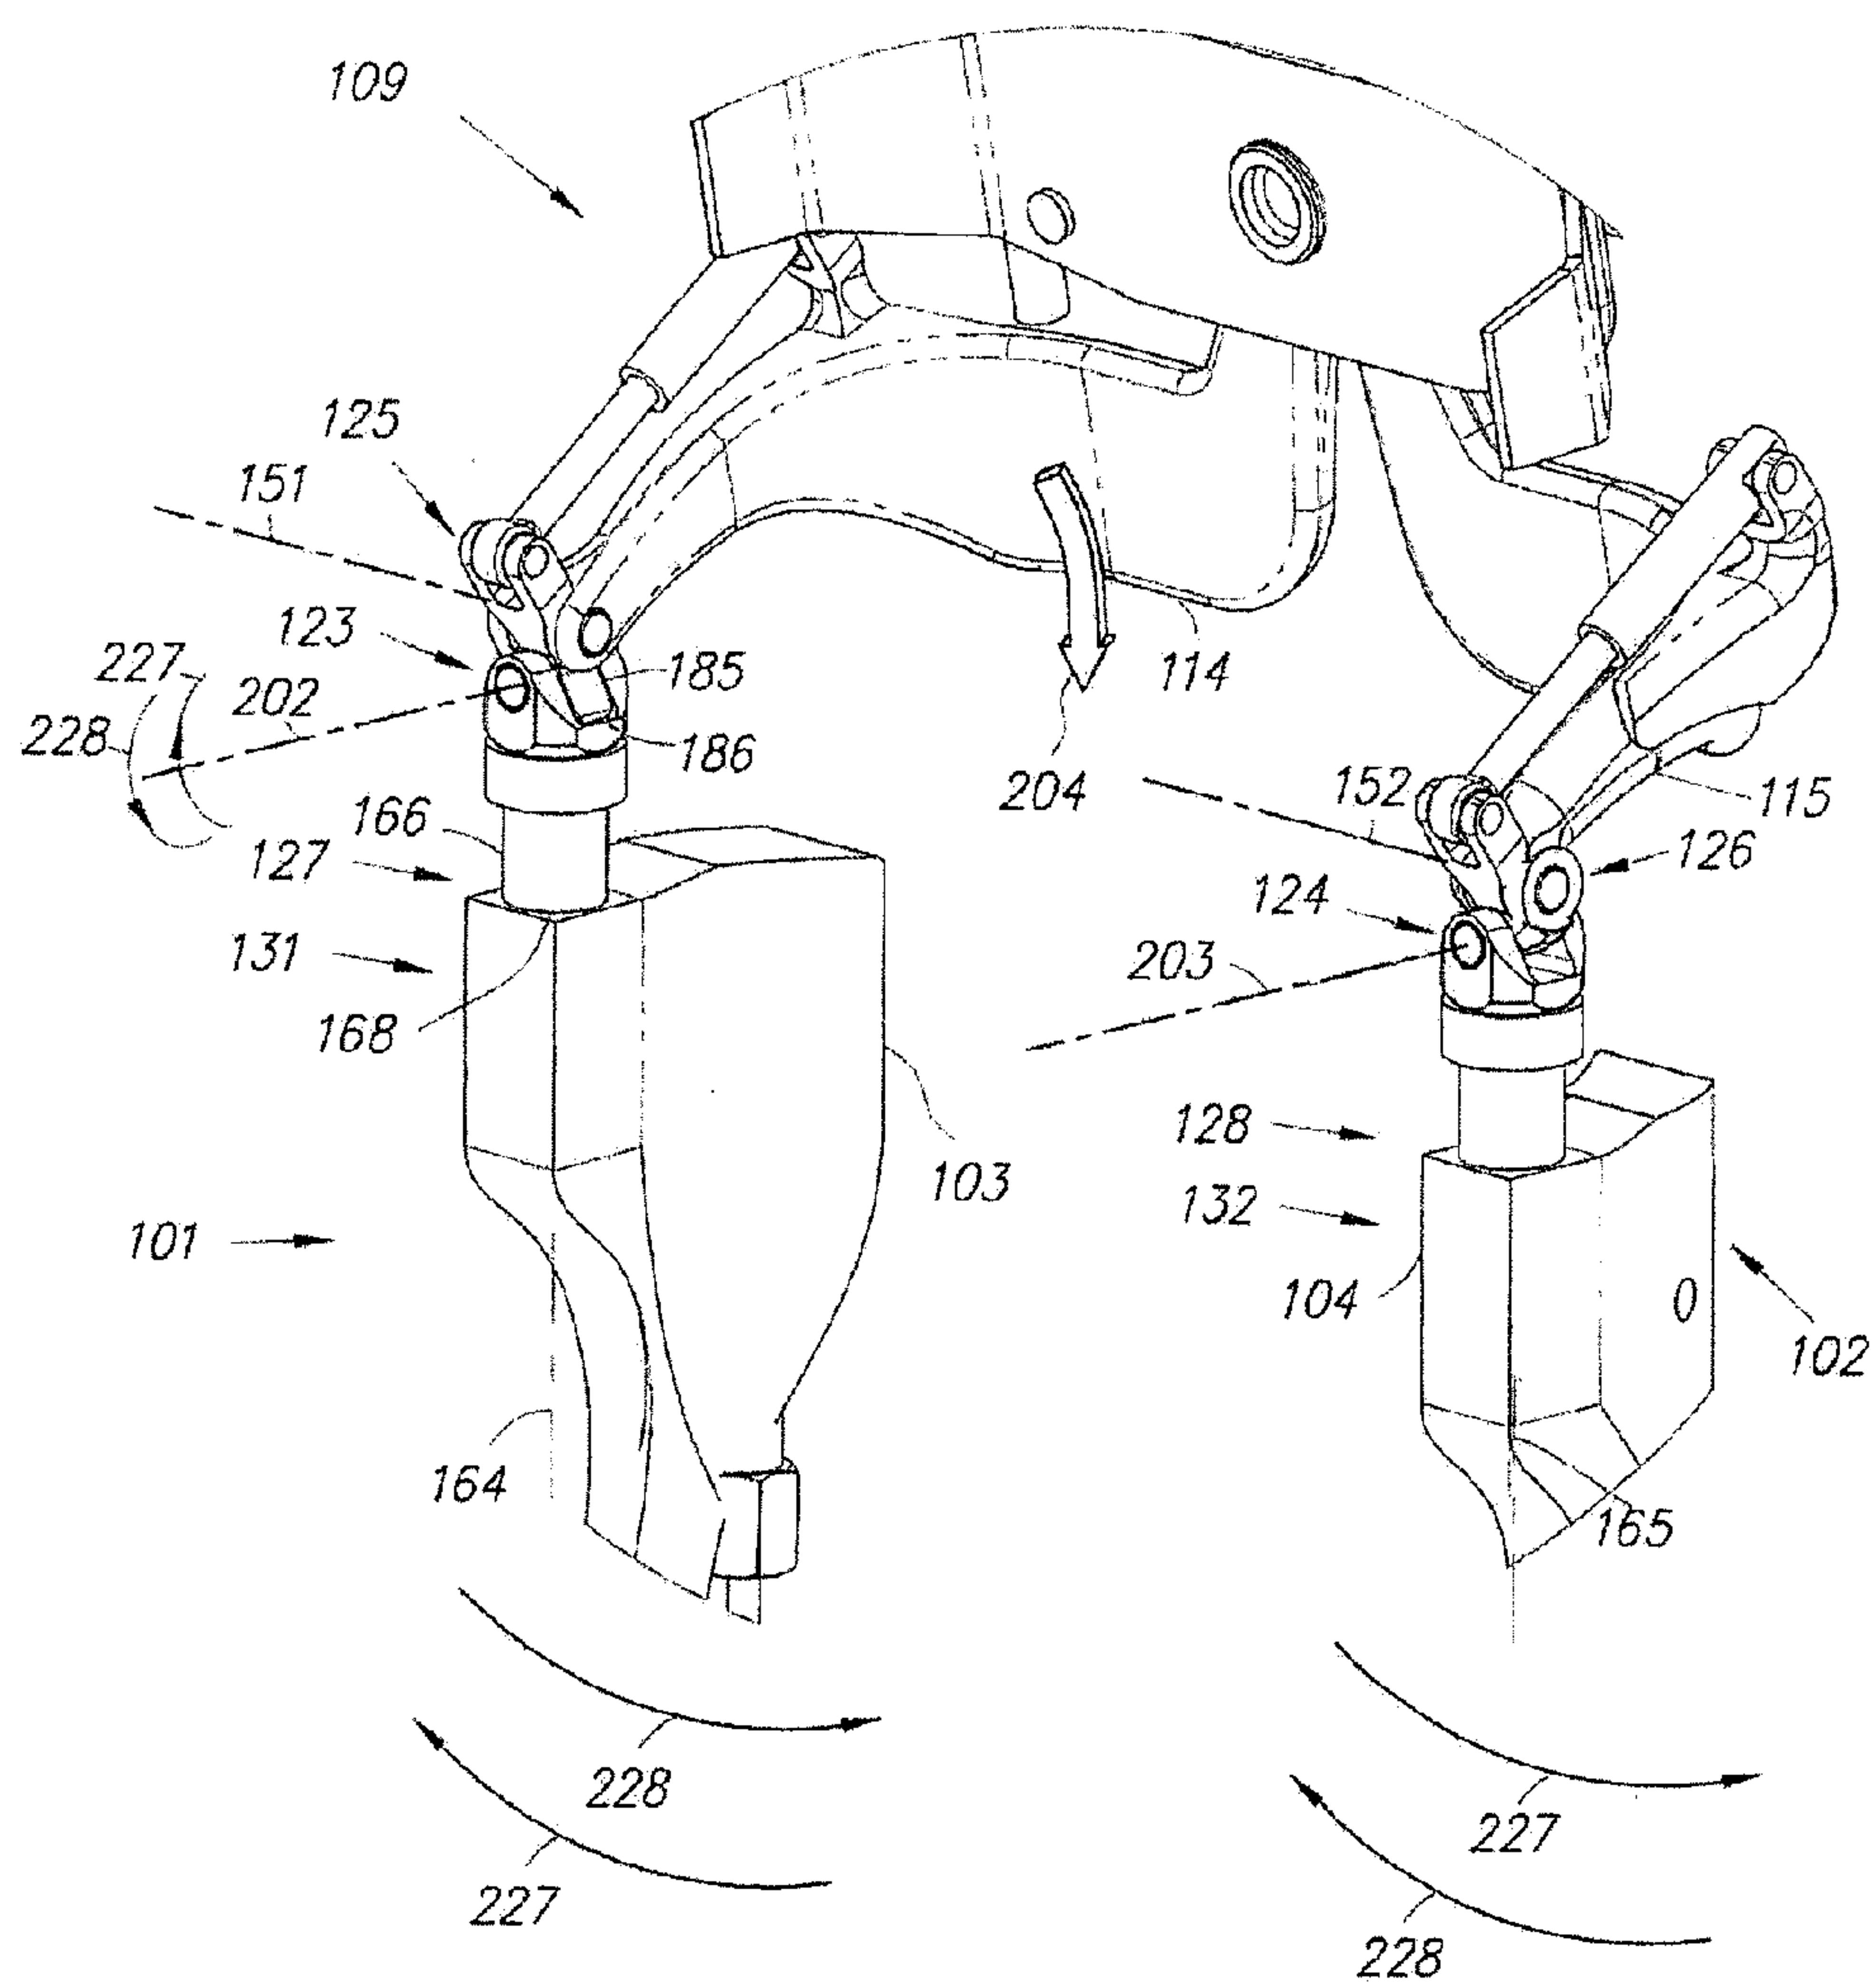
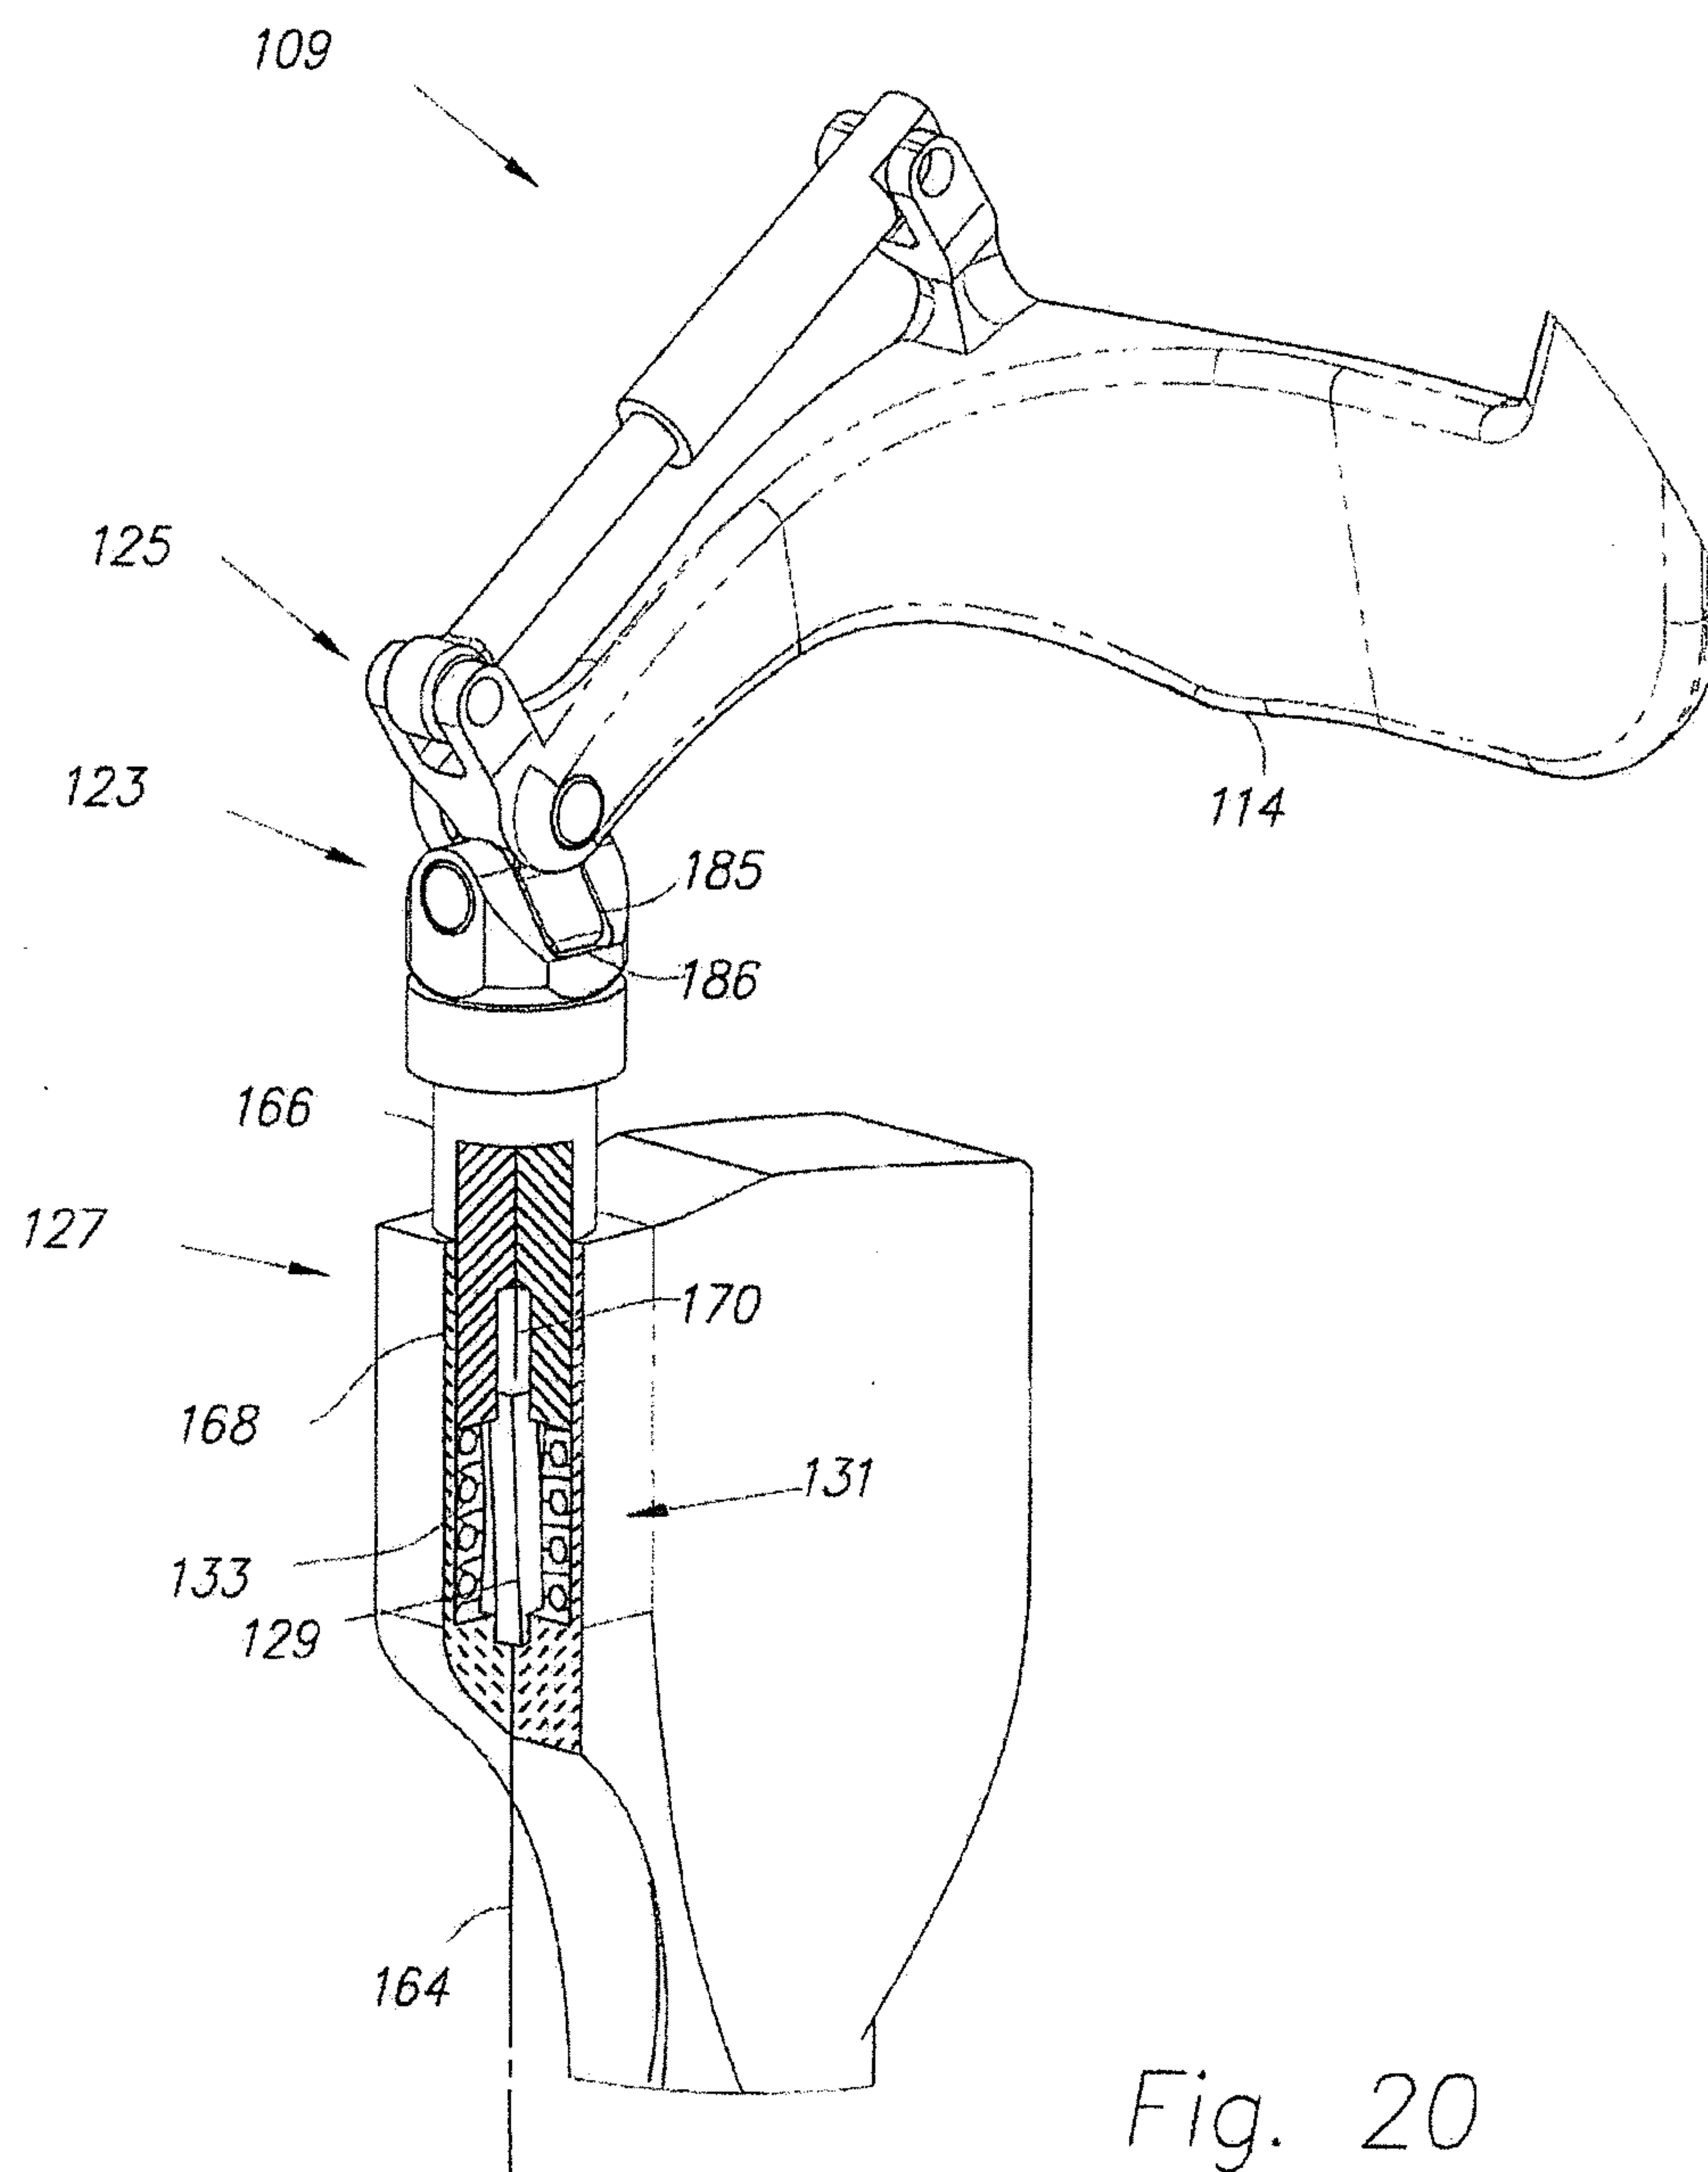


Fig. 19



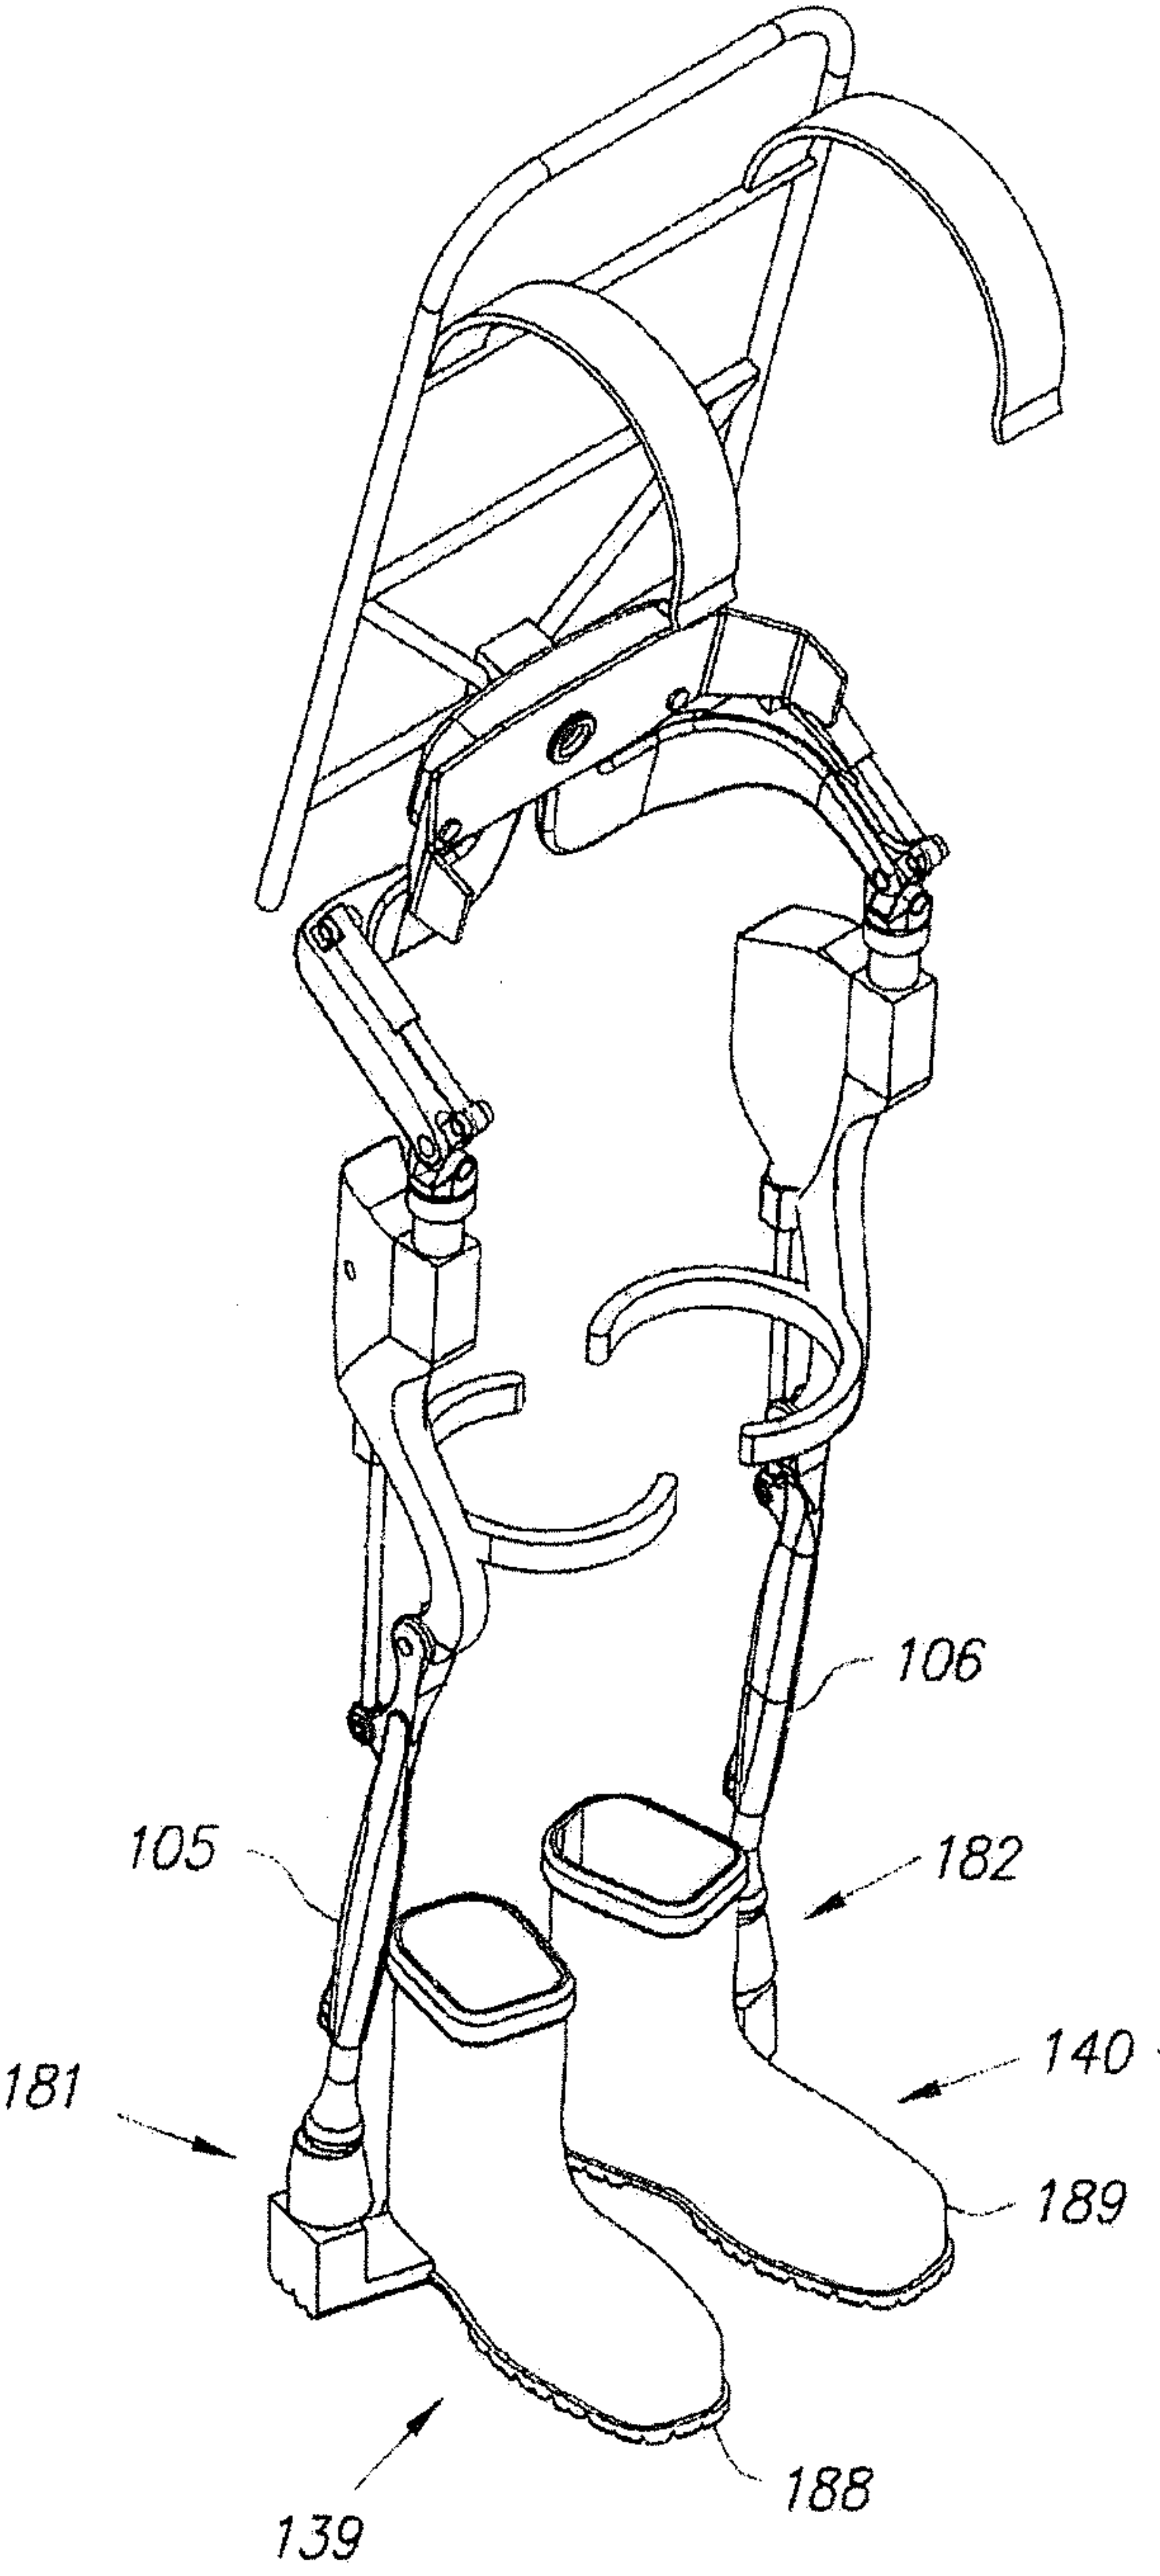


Fig. 21

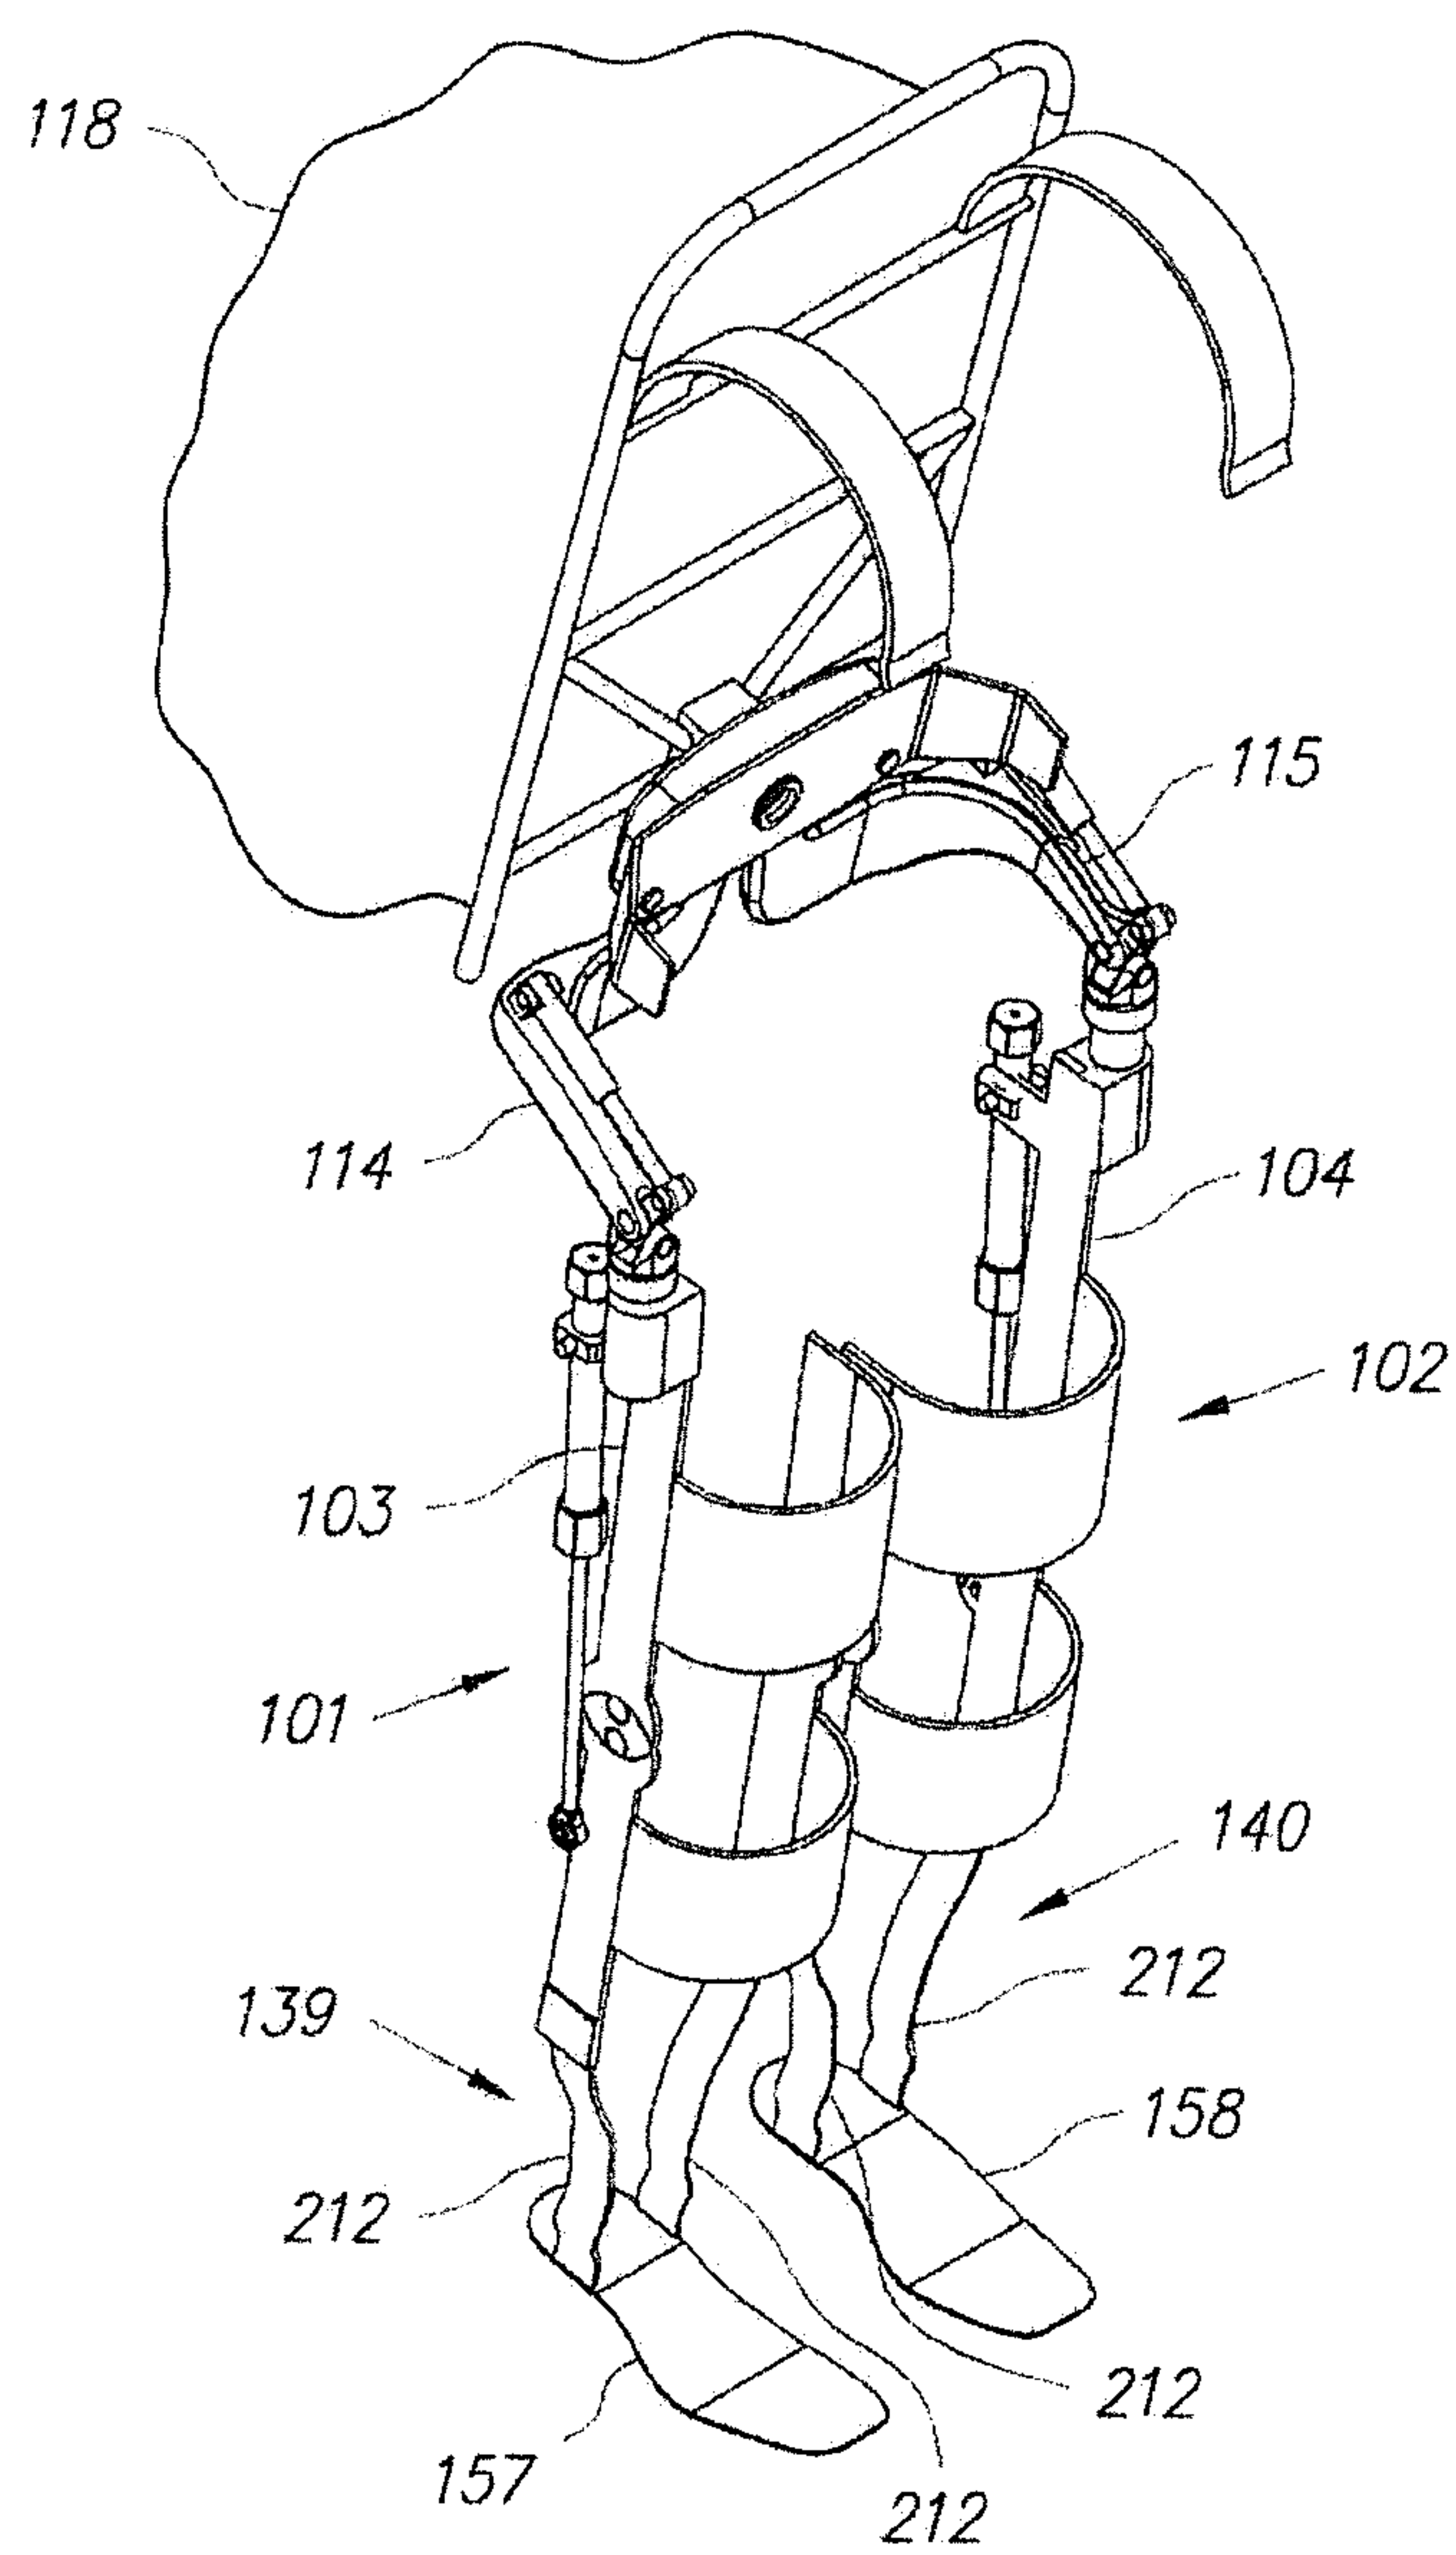


Fig. 22

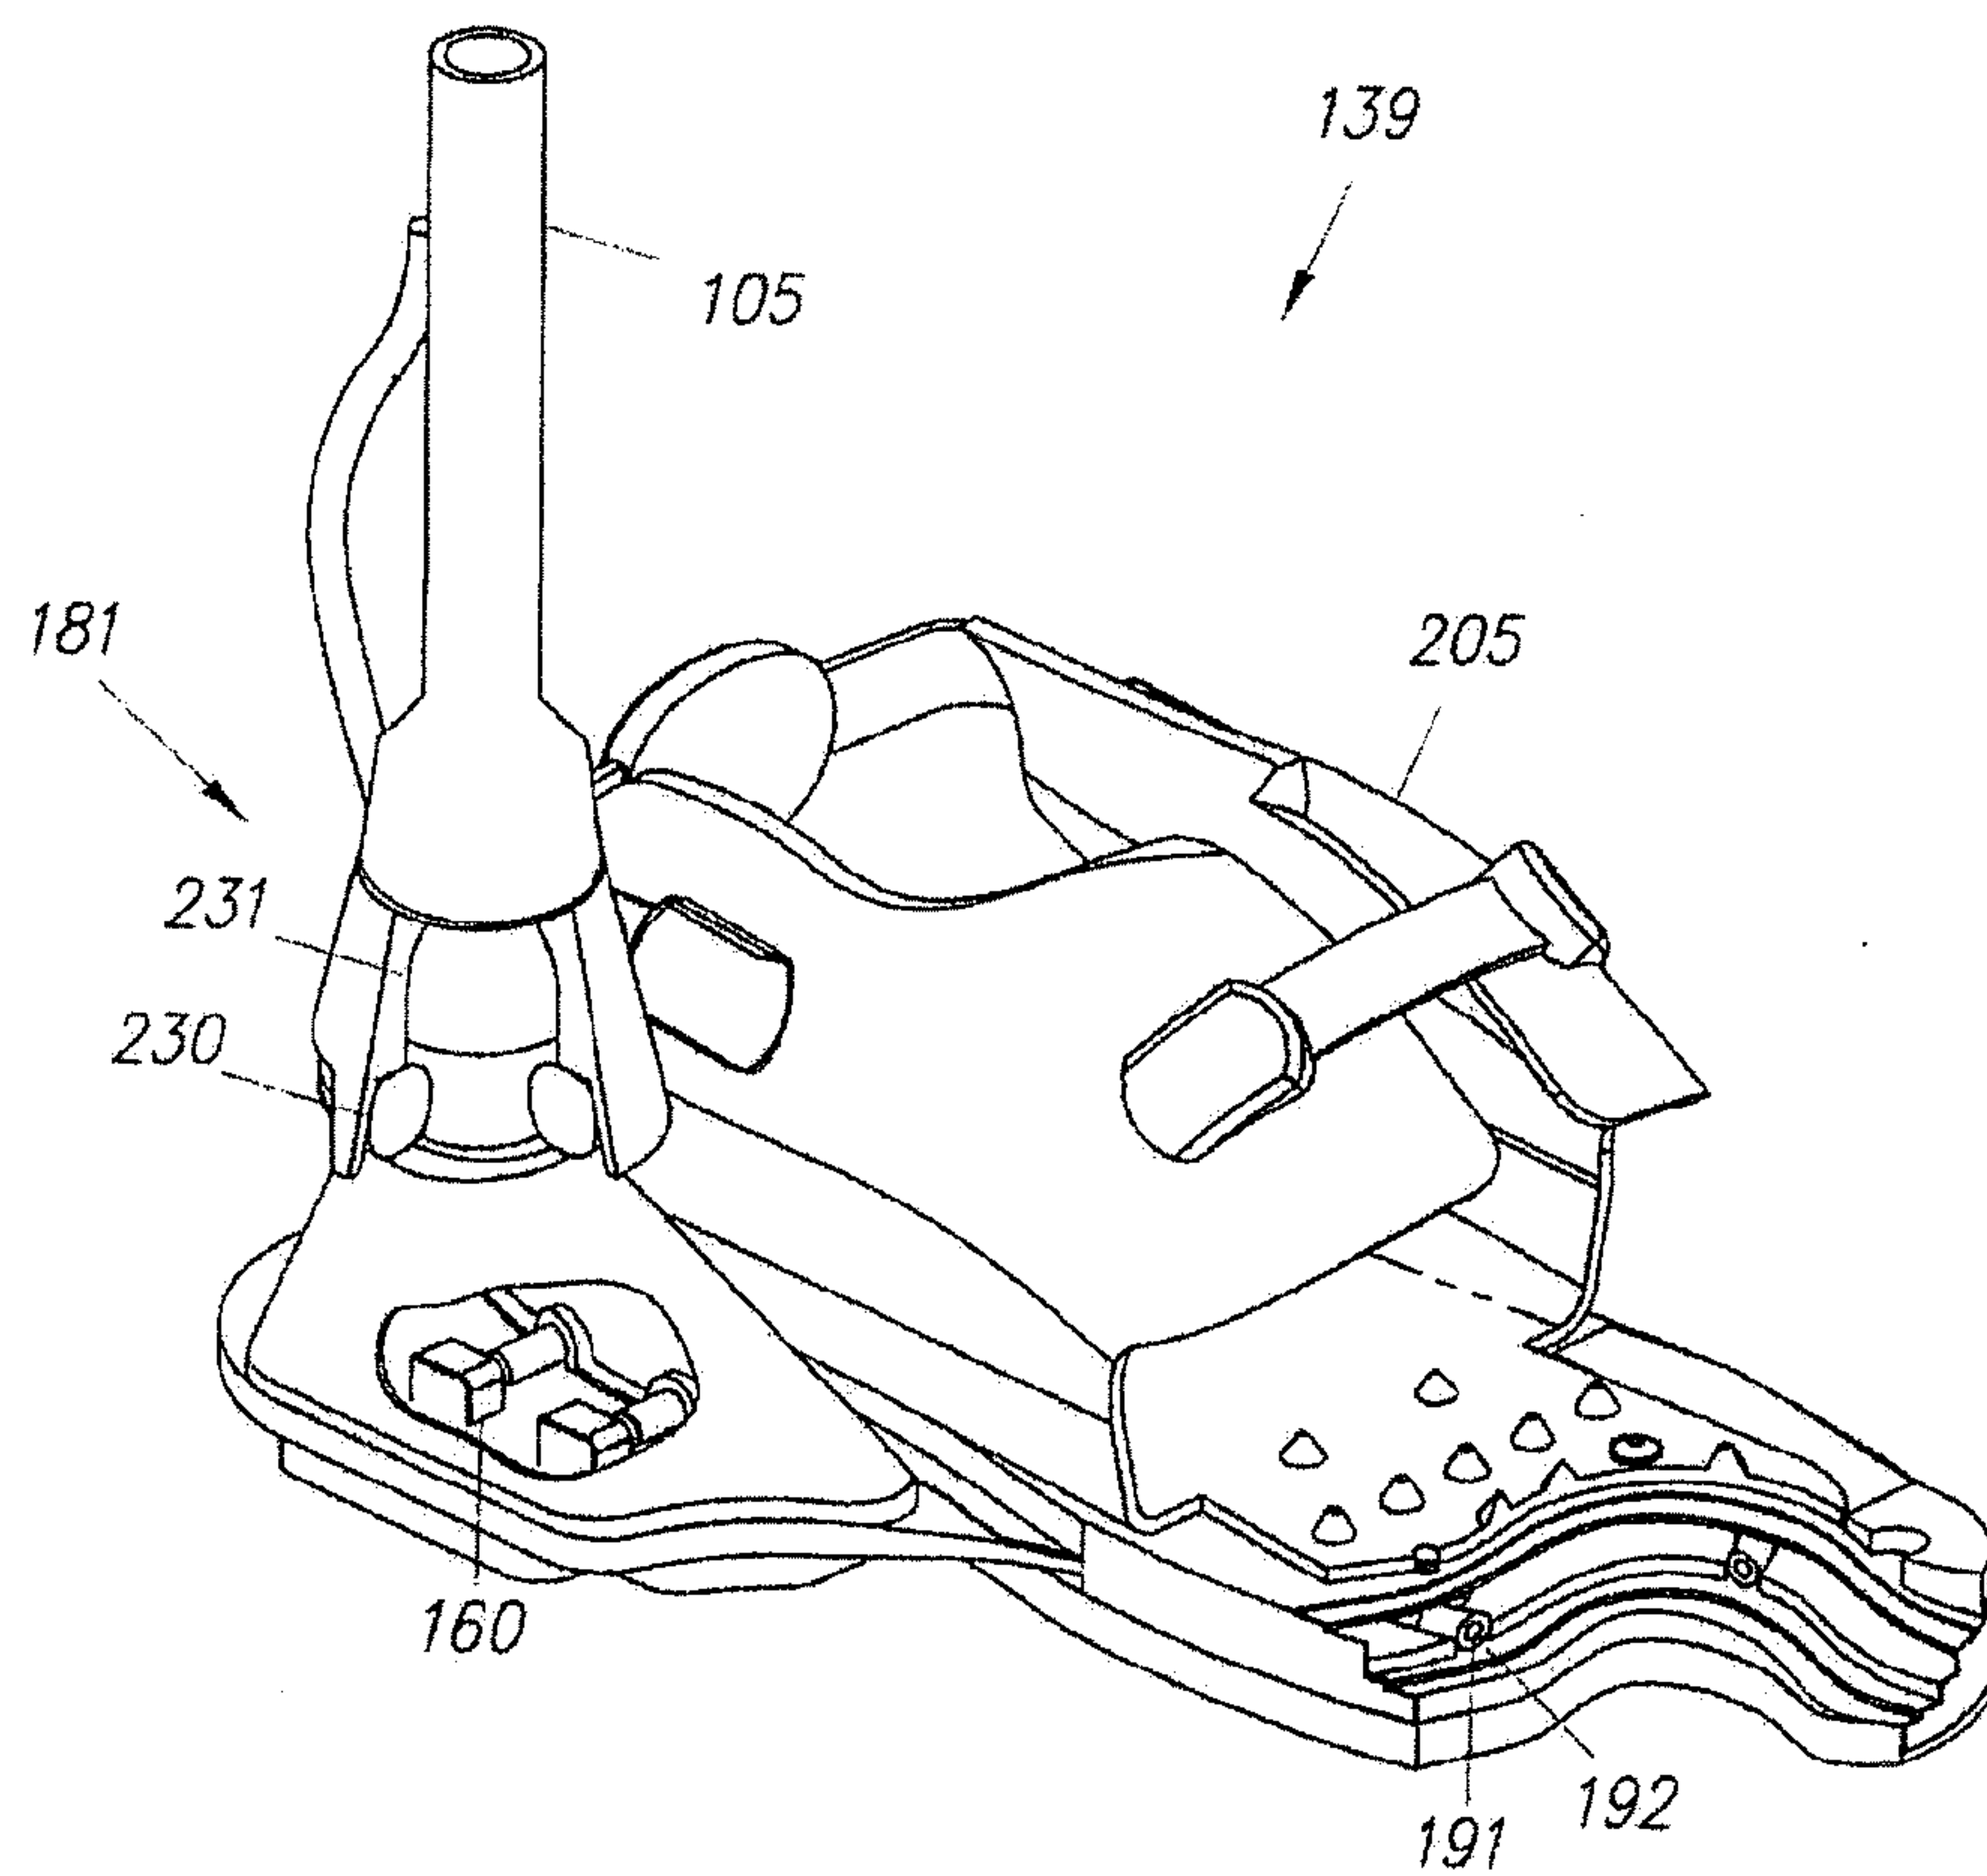


Fig. 23

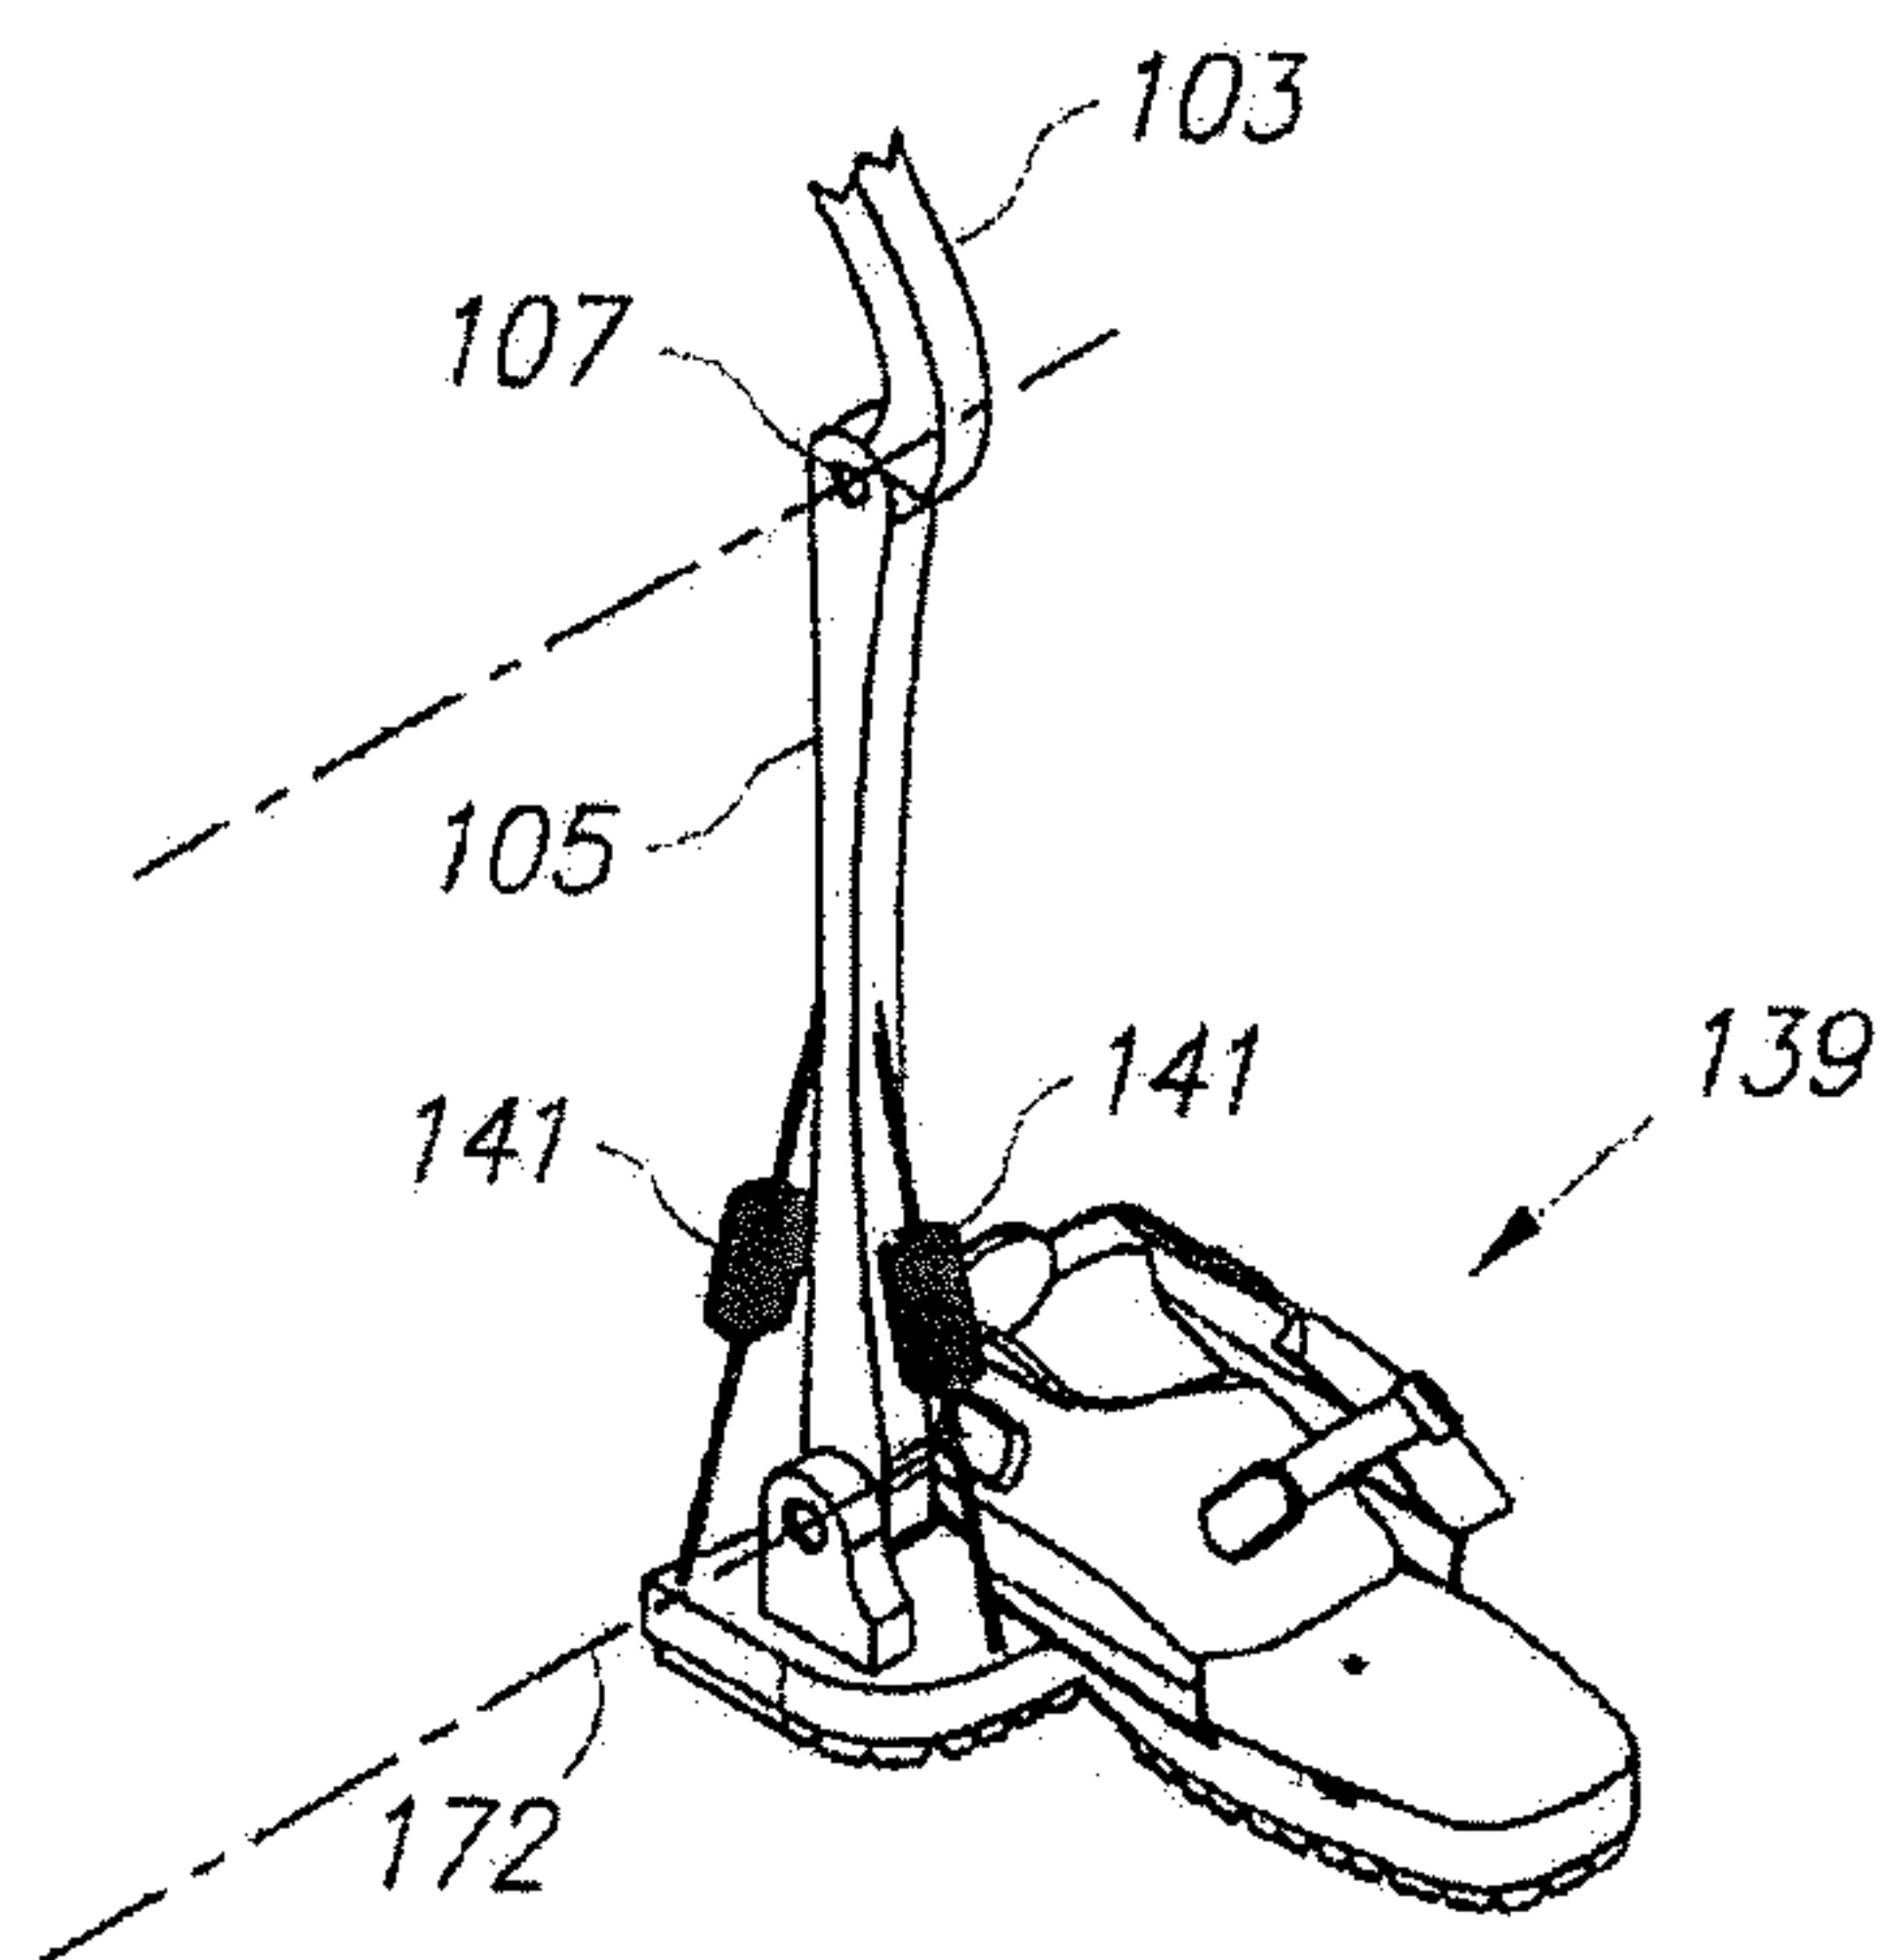


Fig. 24

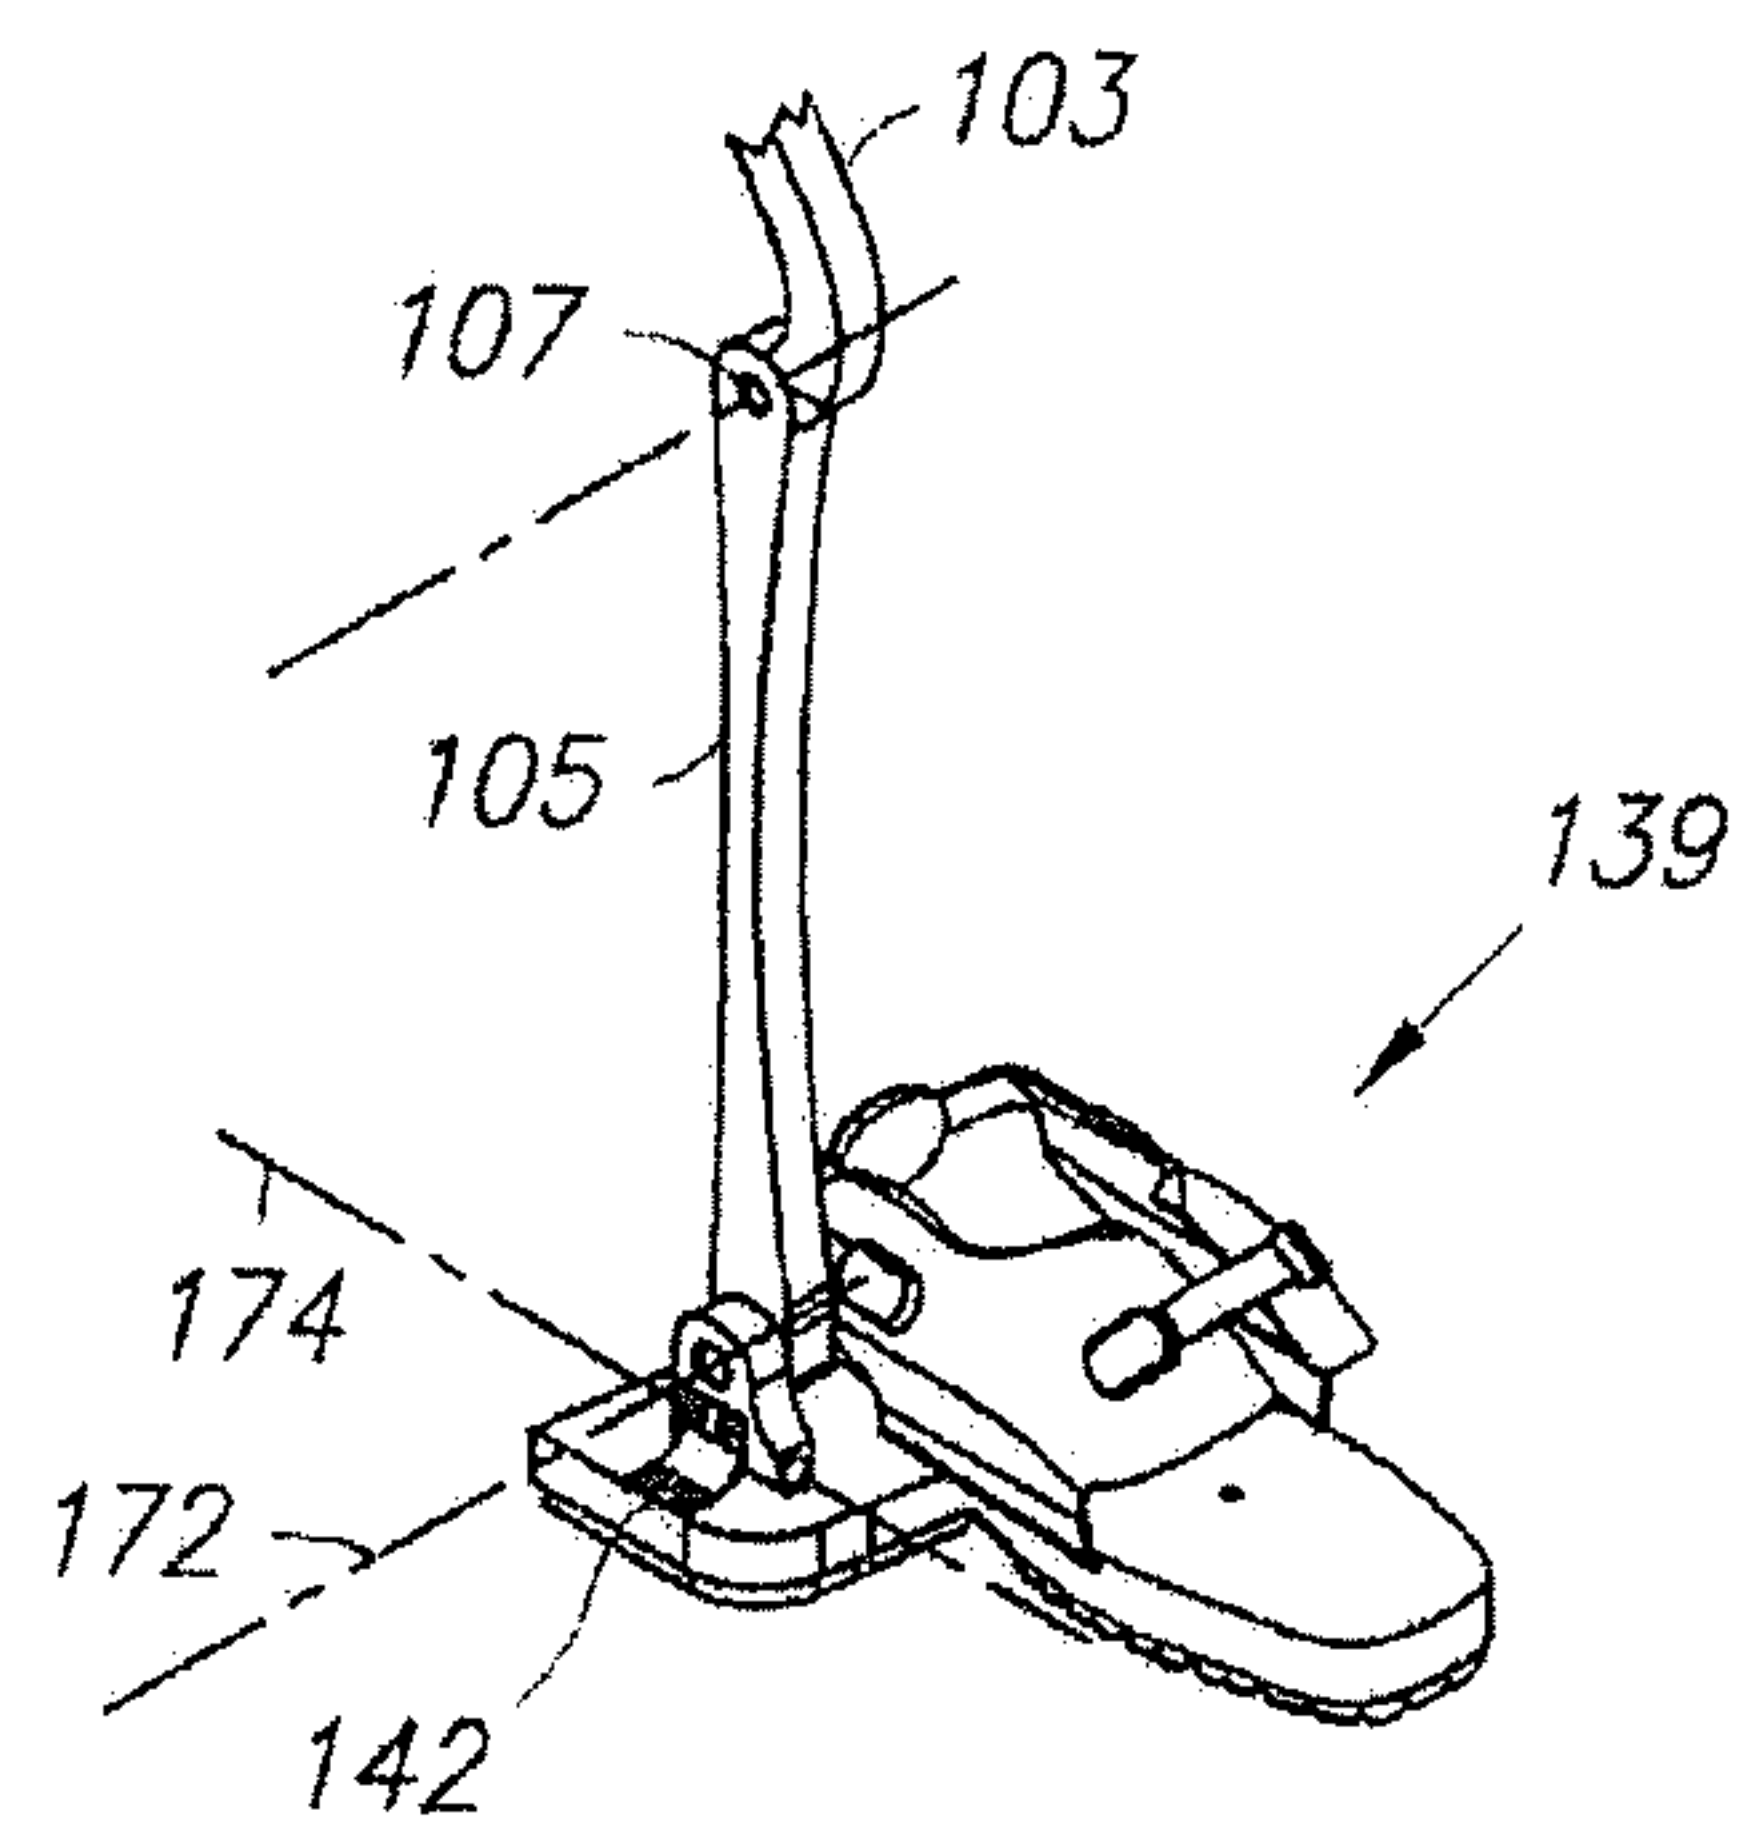


Fig. 25

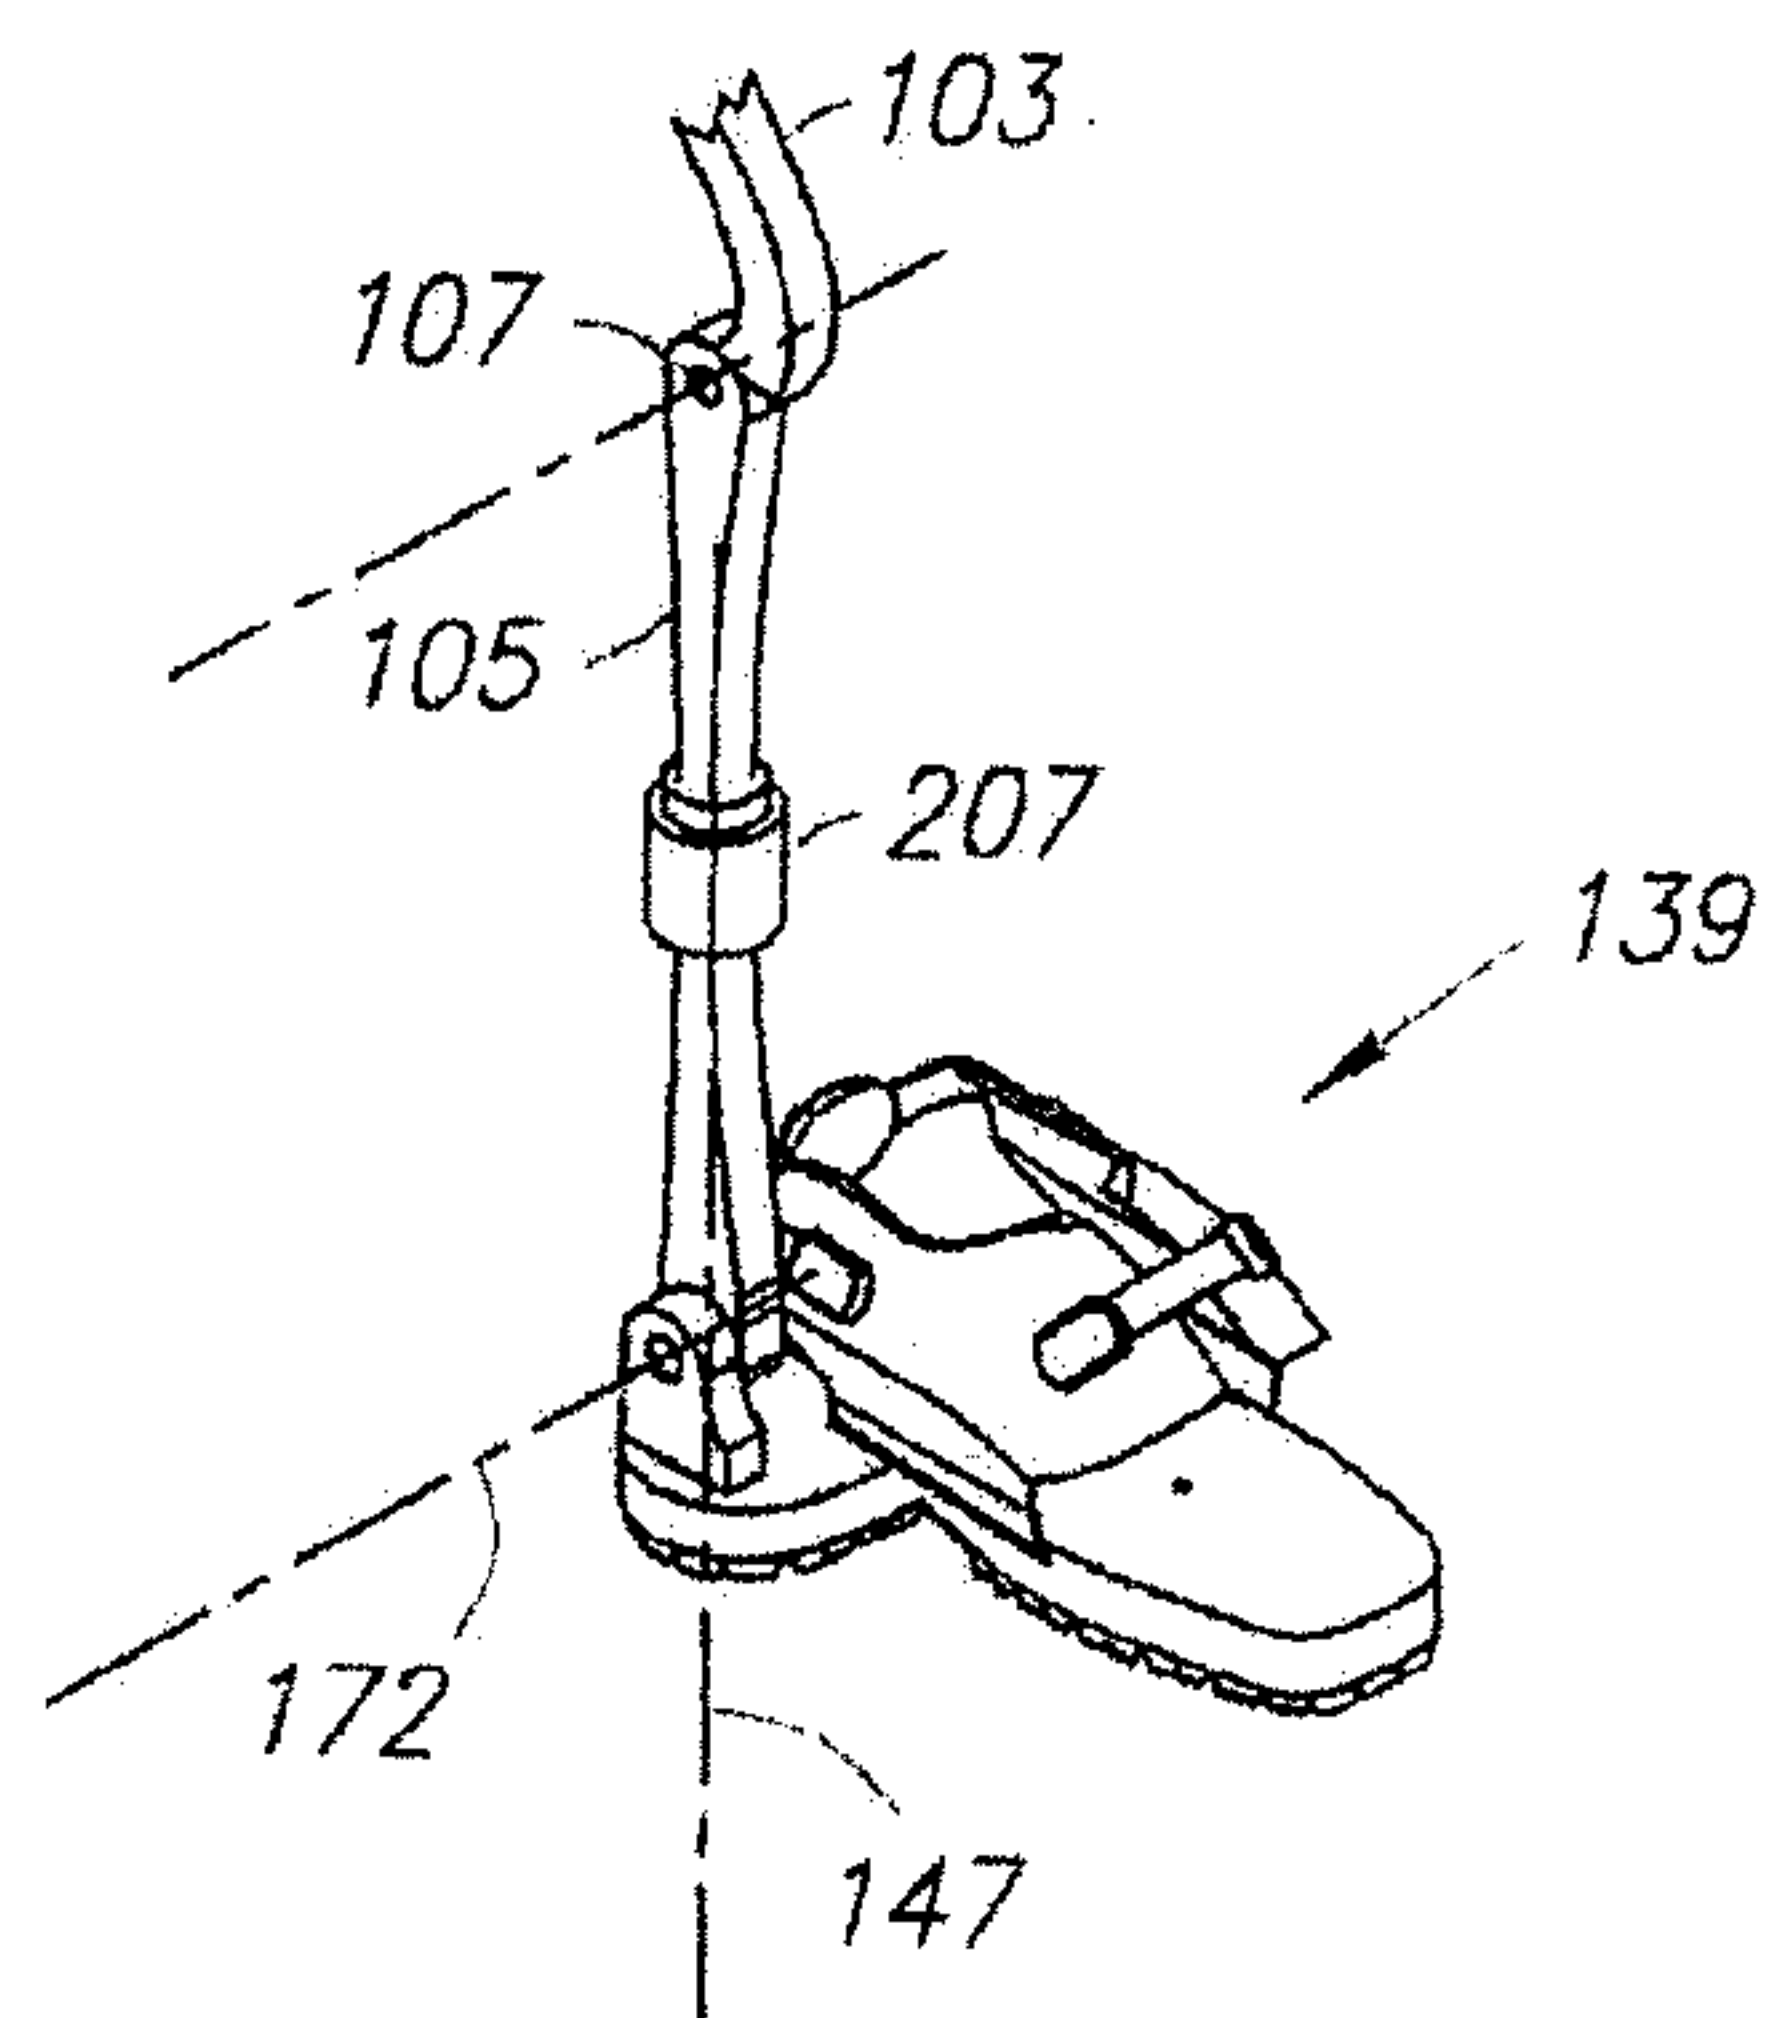


Fig. 26

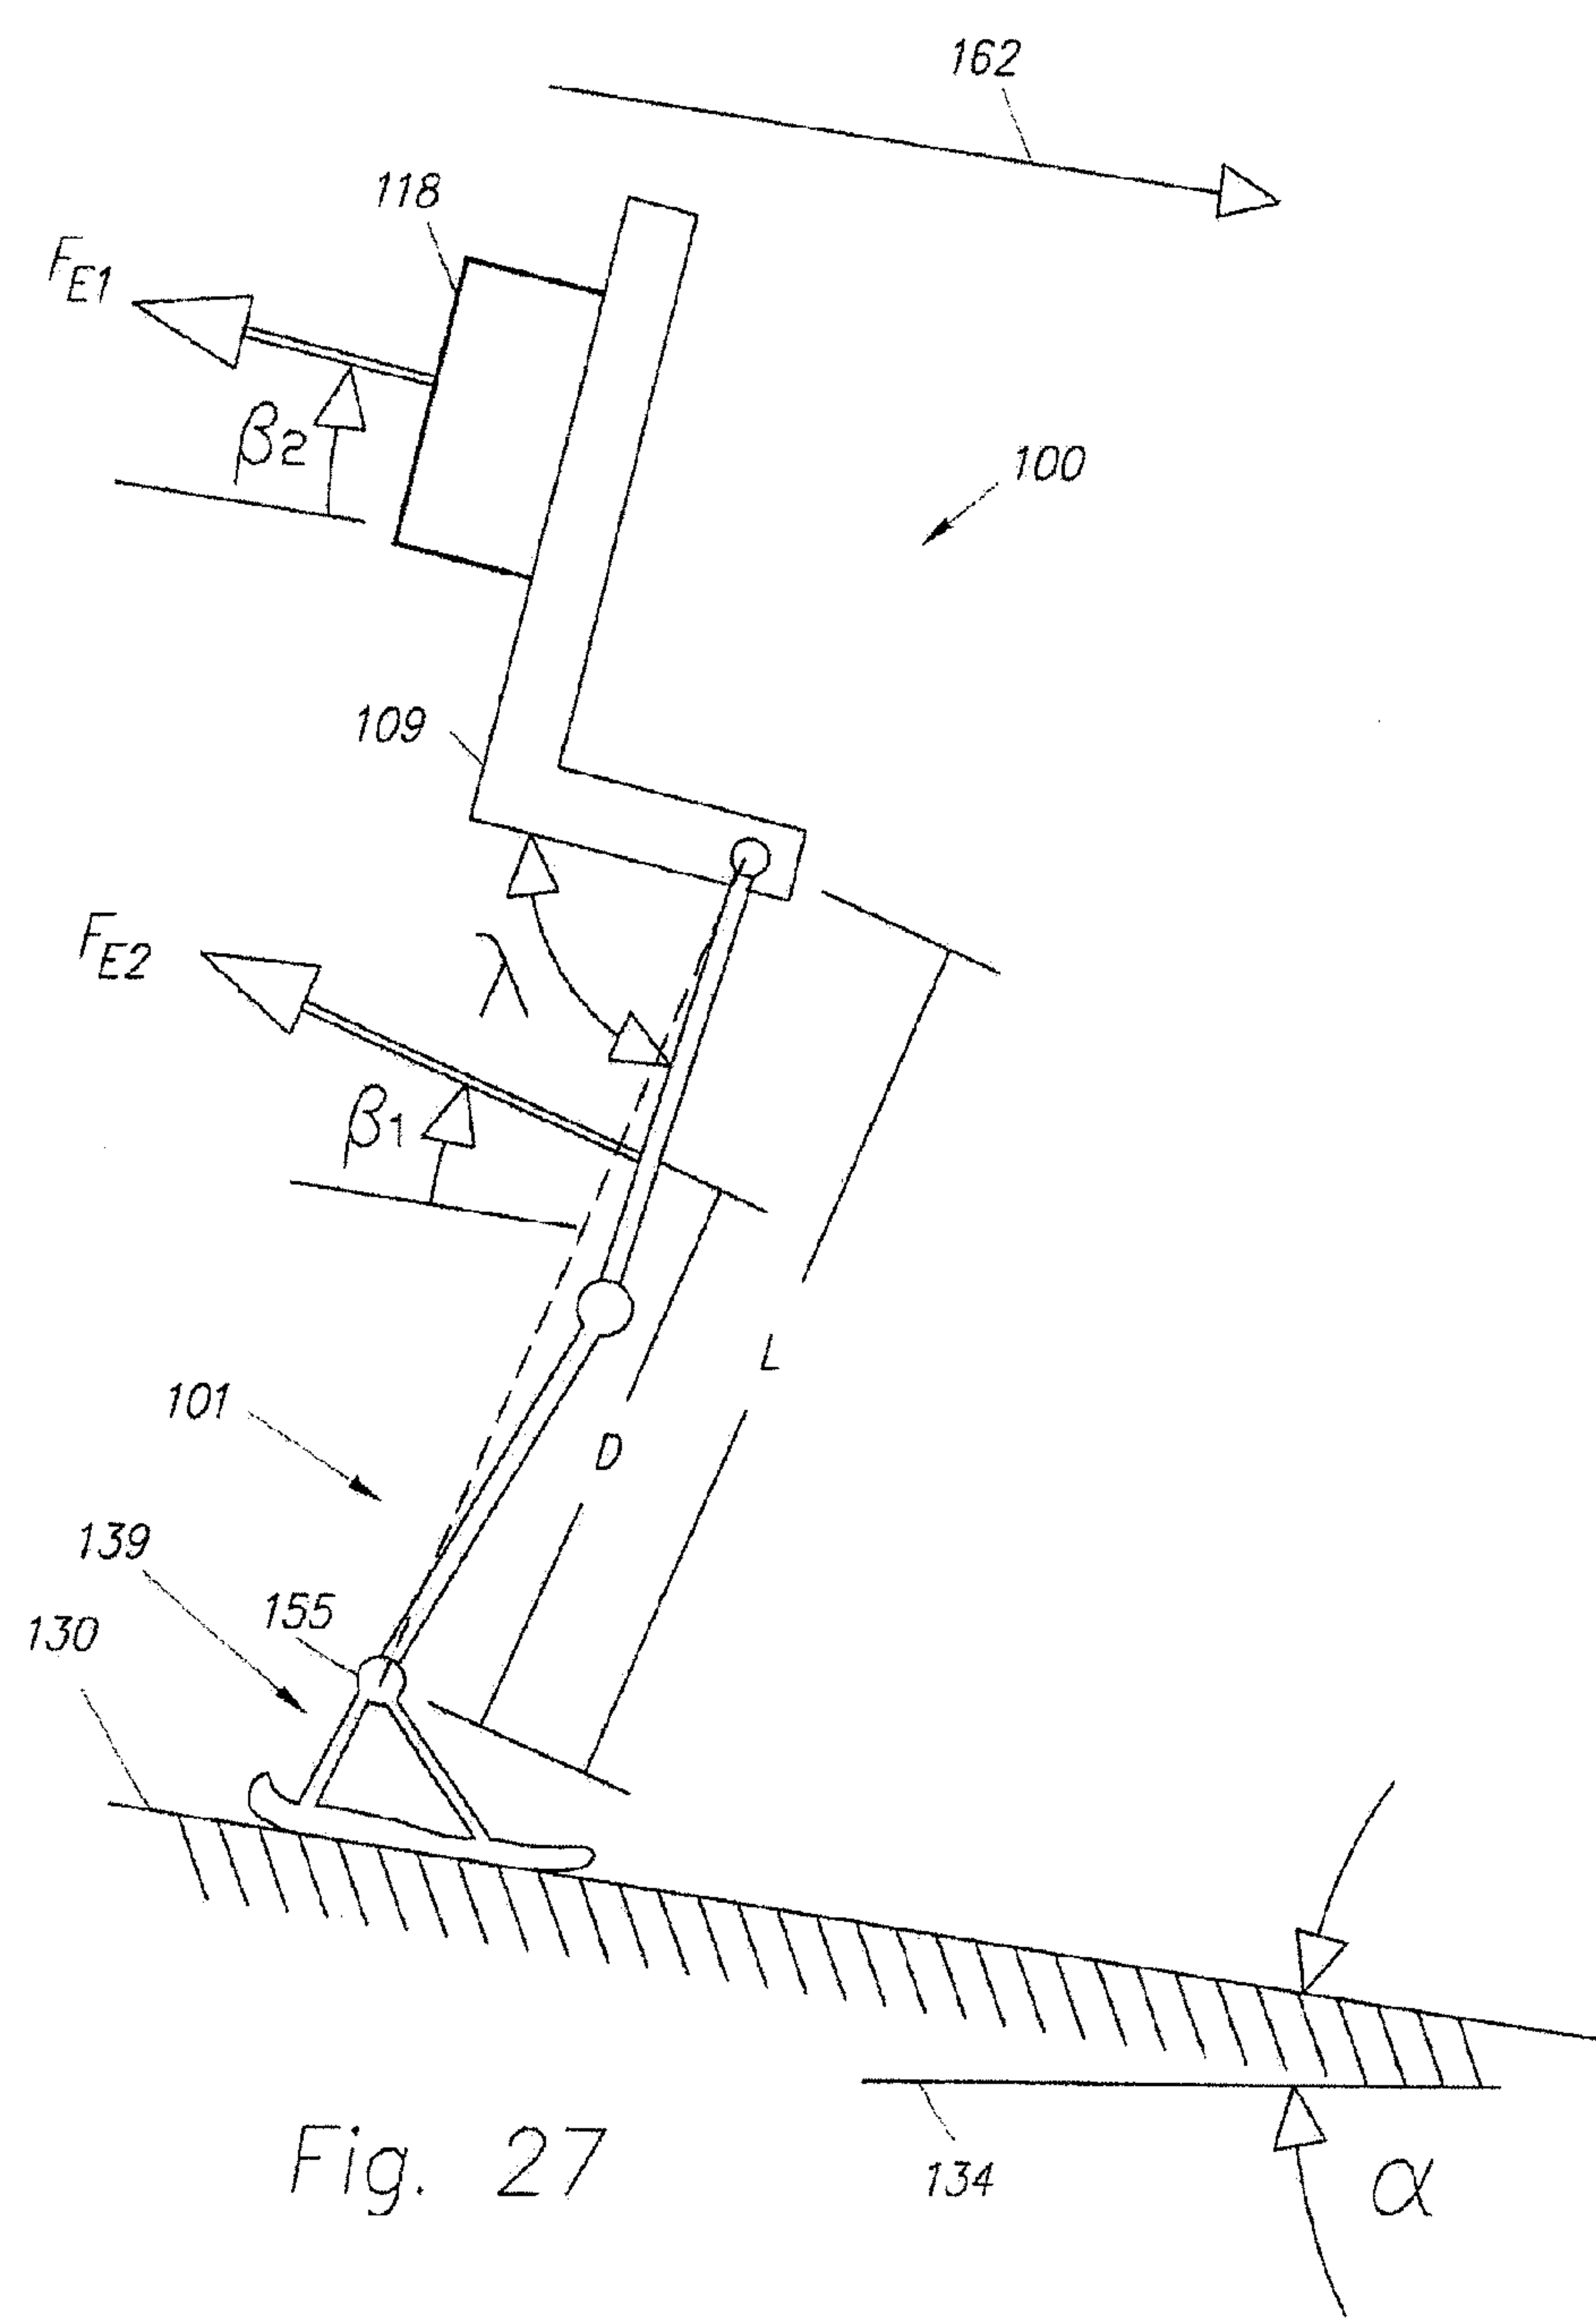


Fig. 27

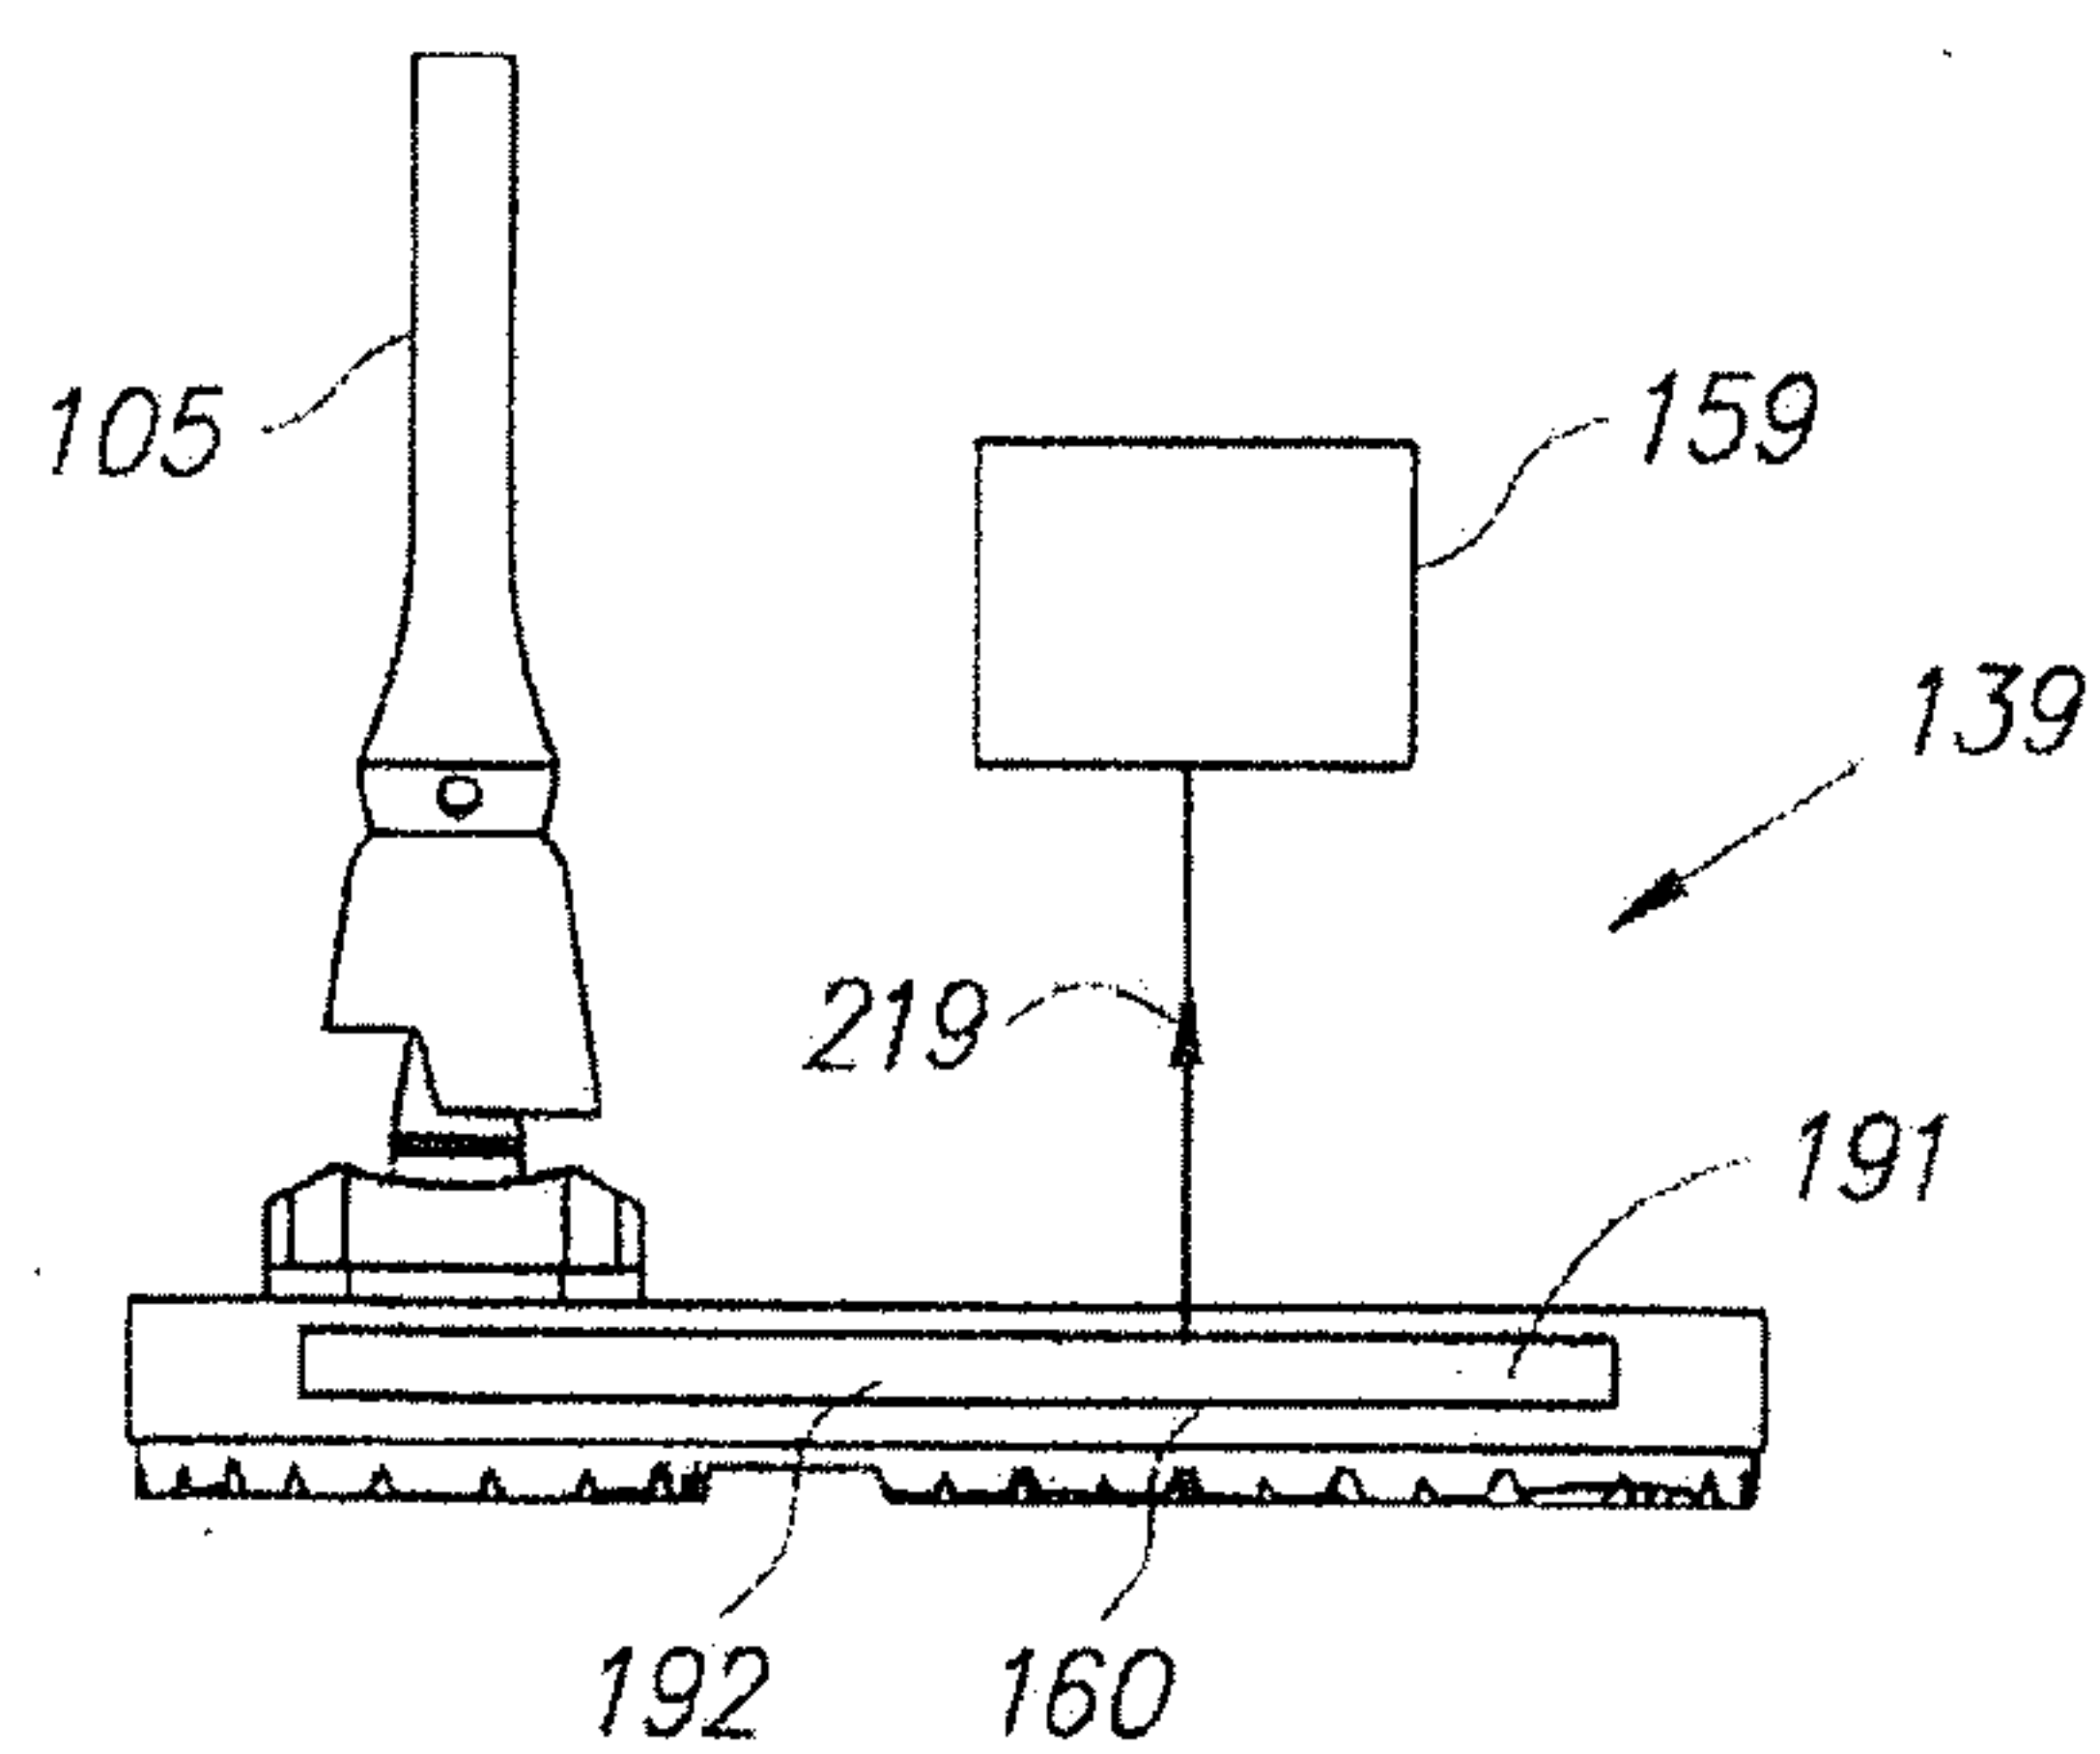


Fig. 28

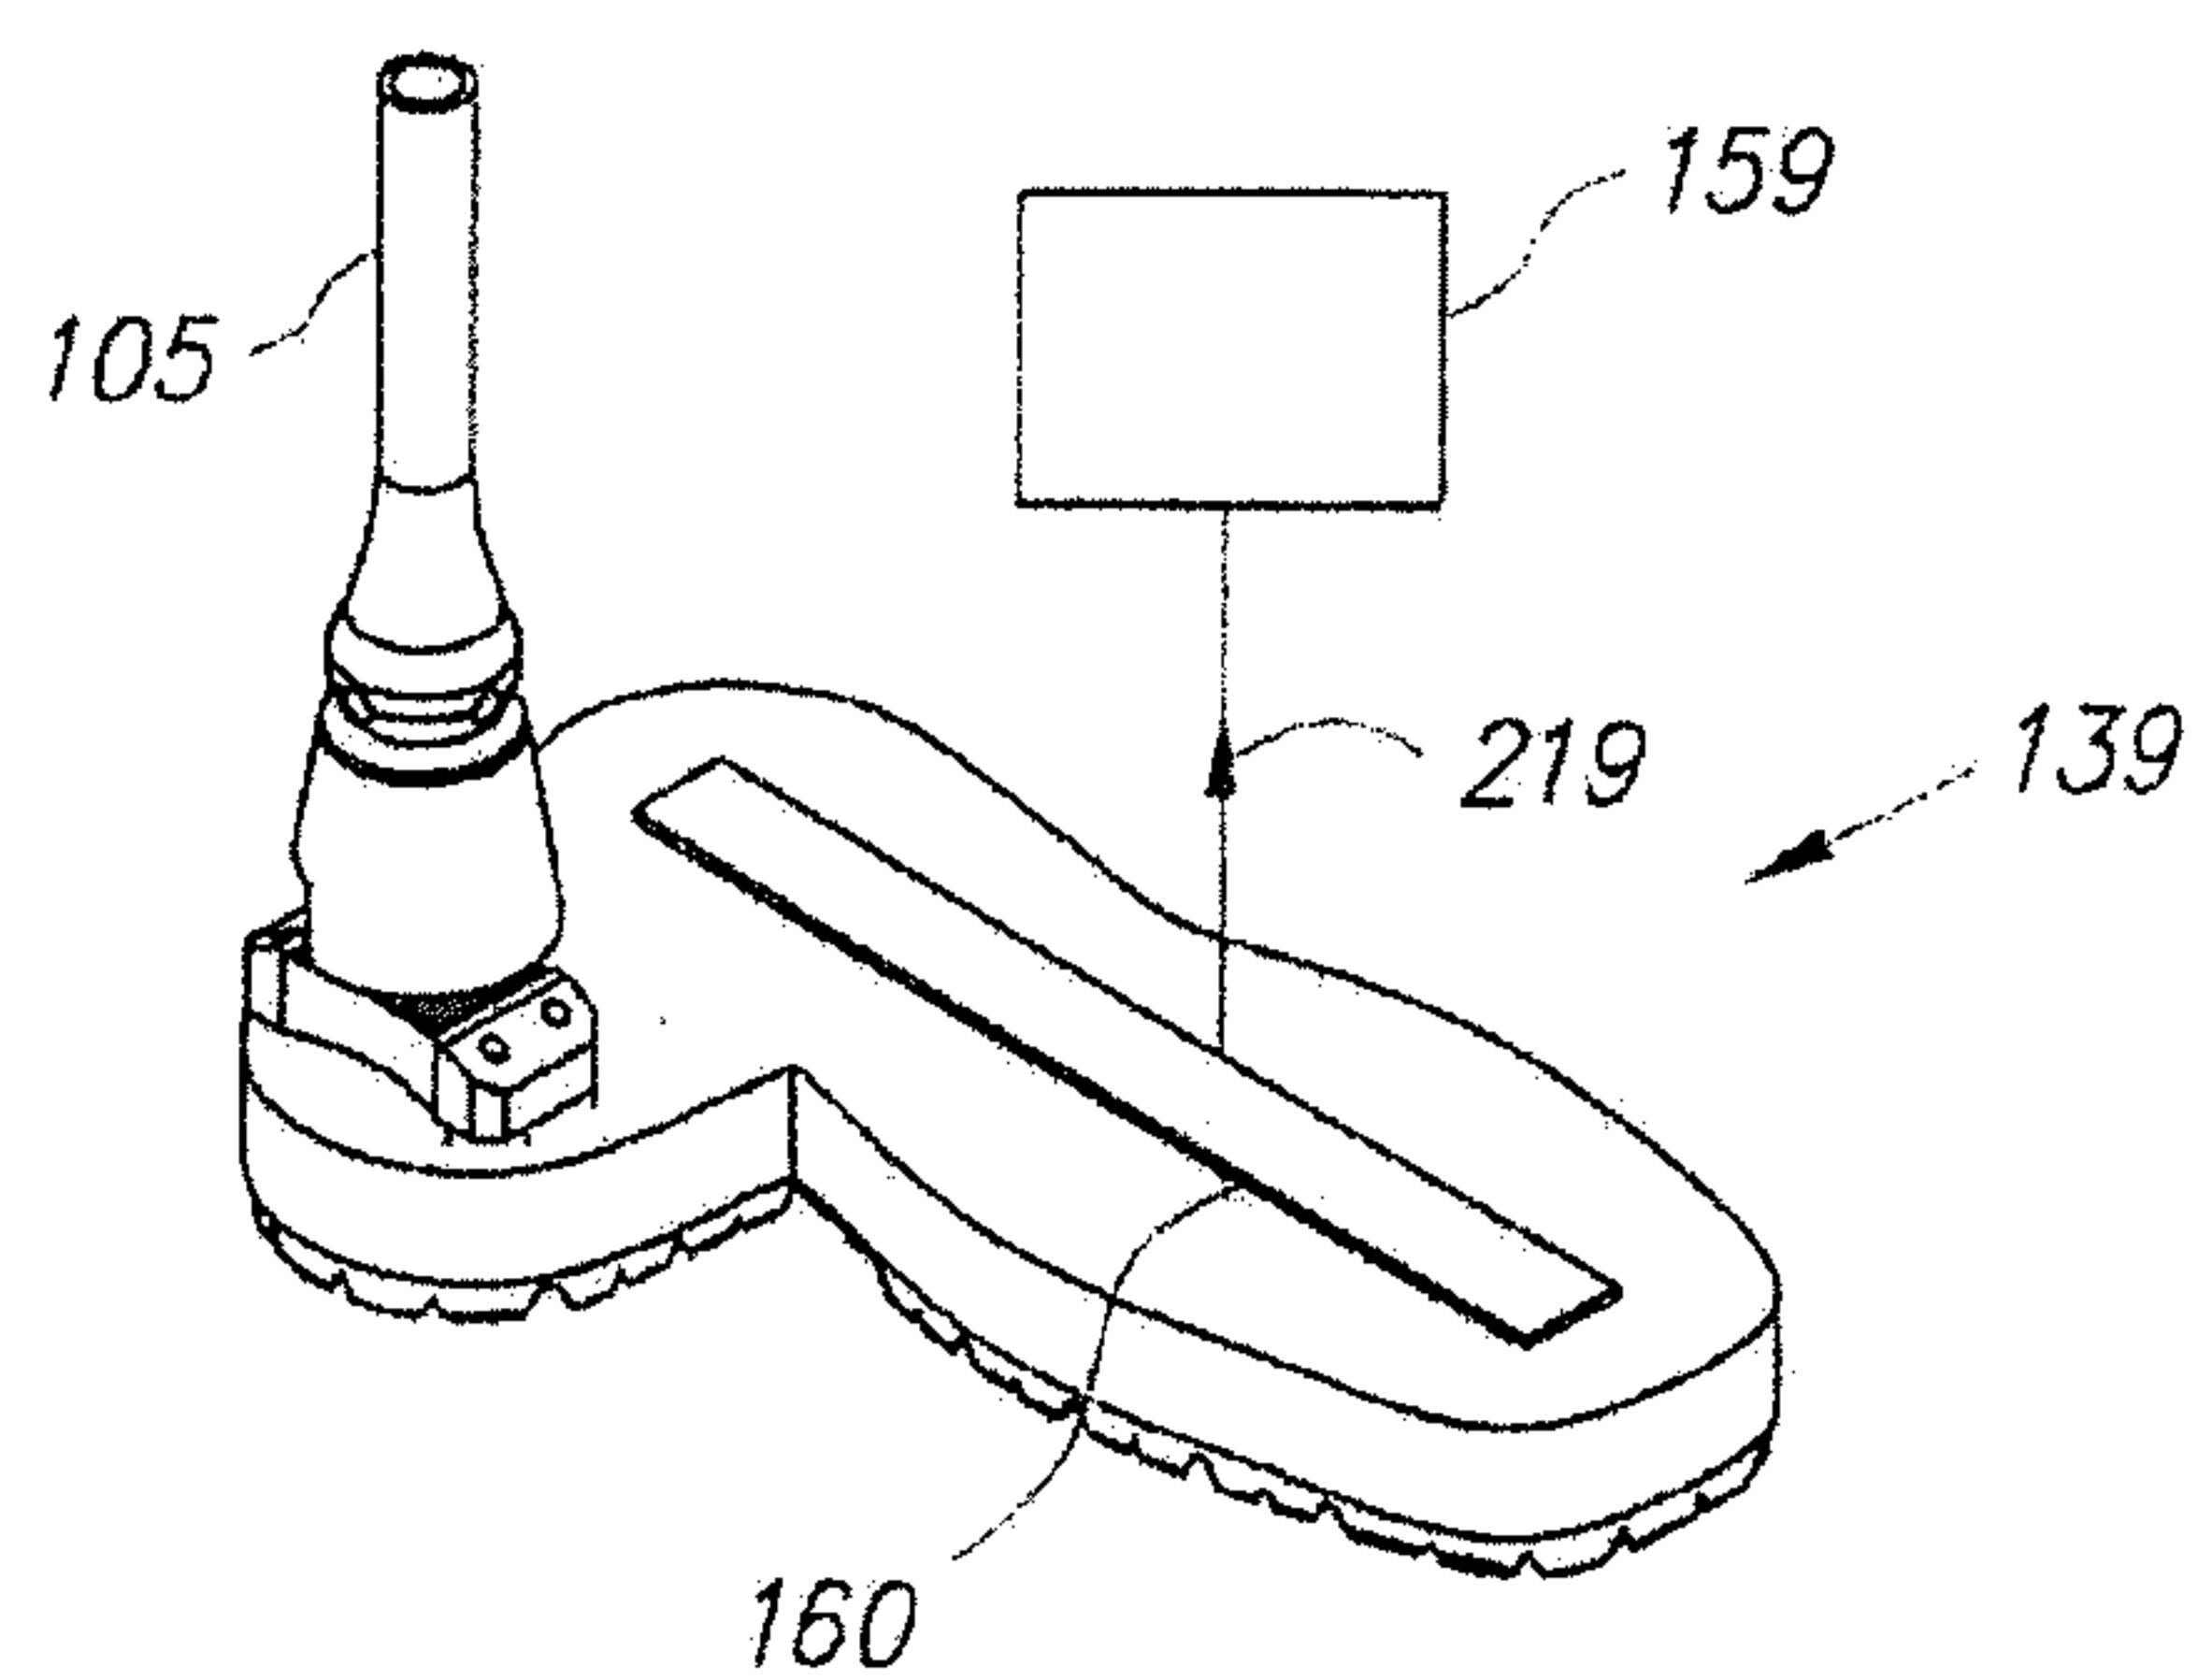


Fig. 29

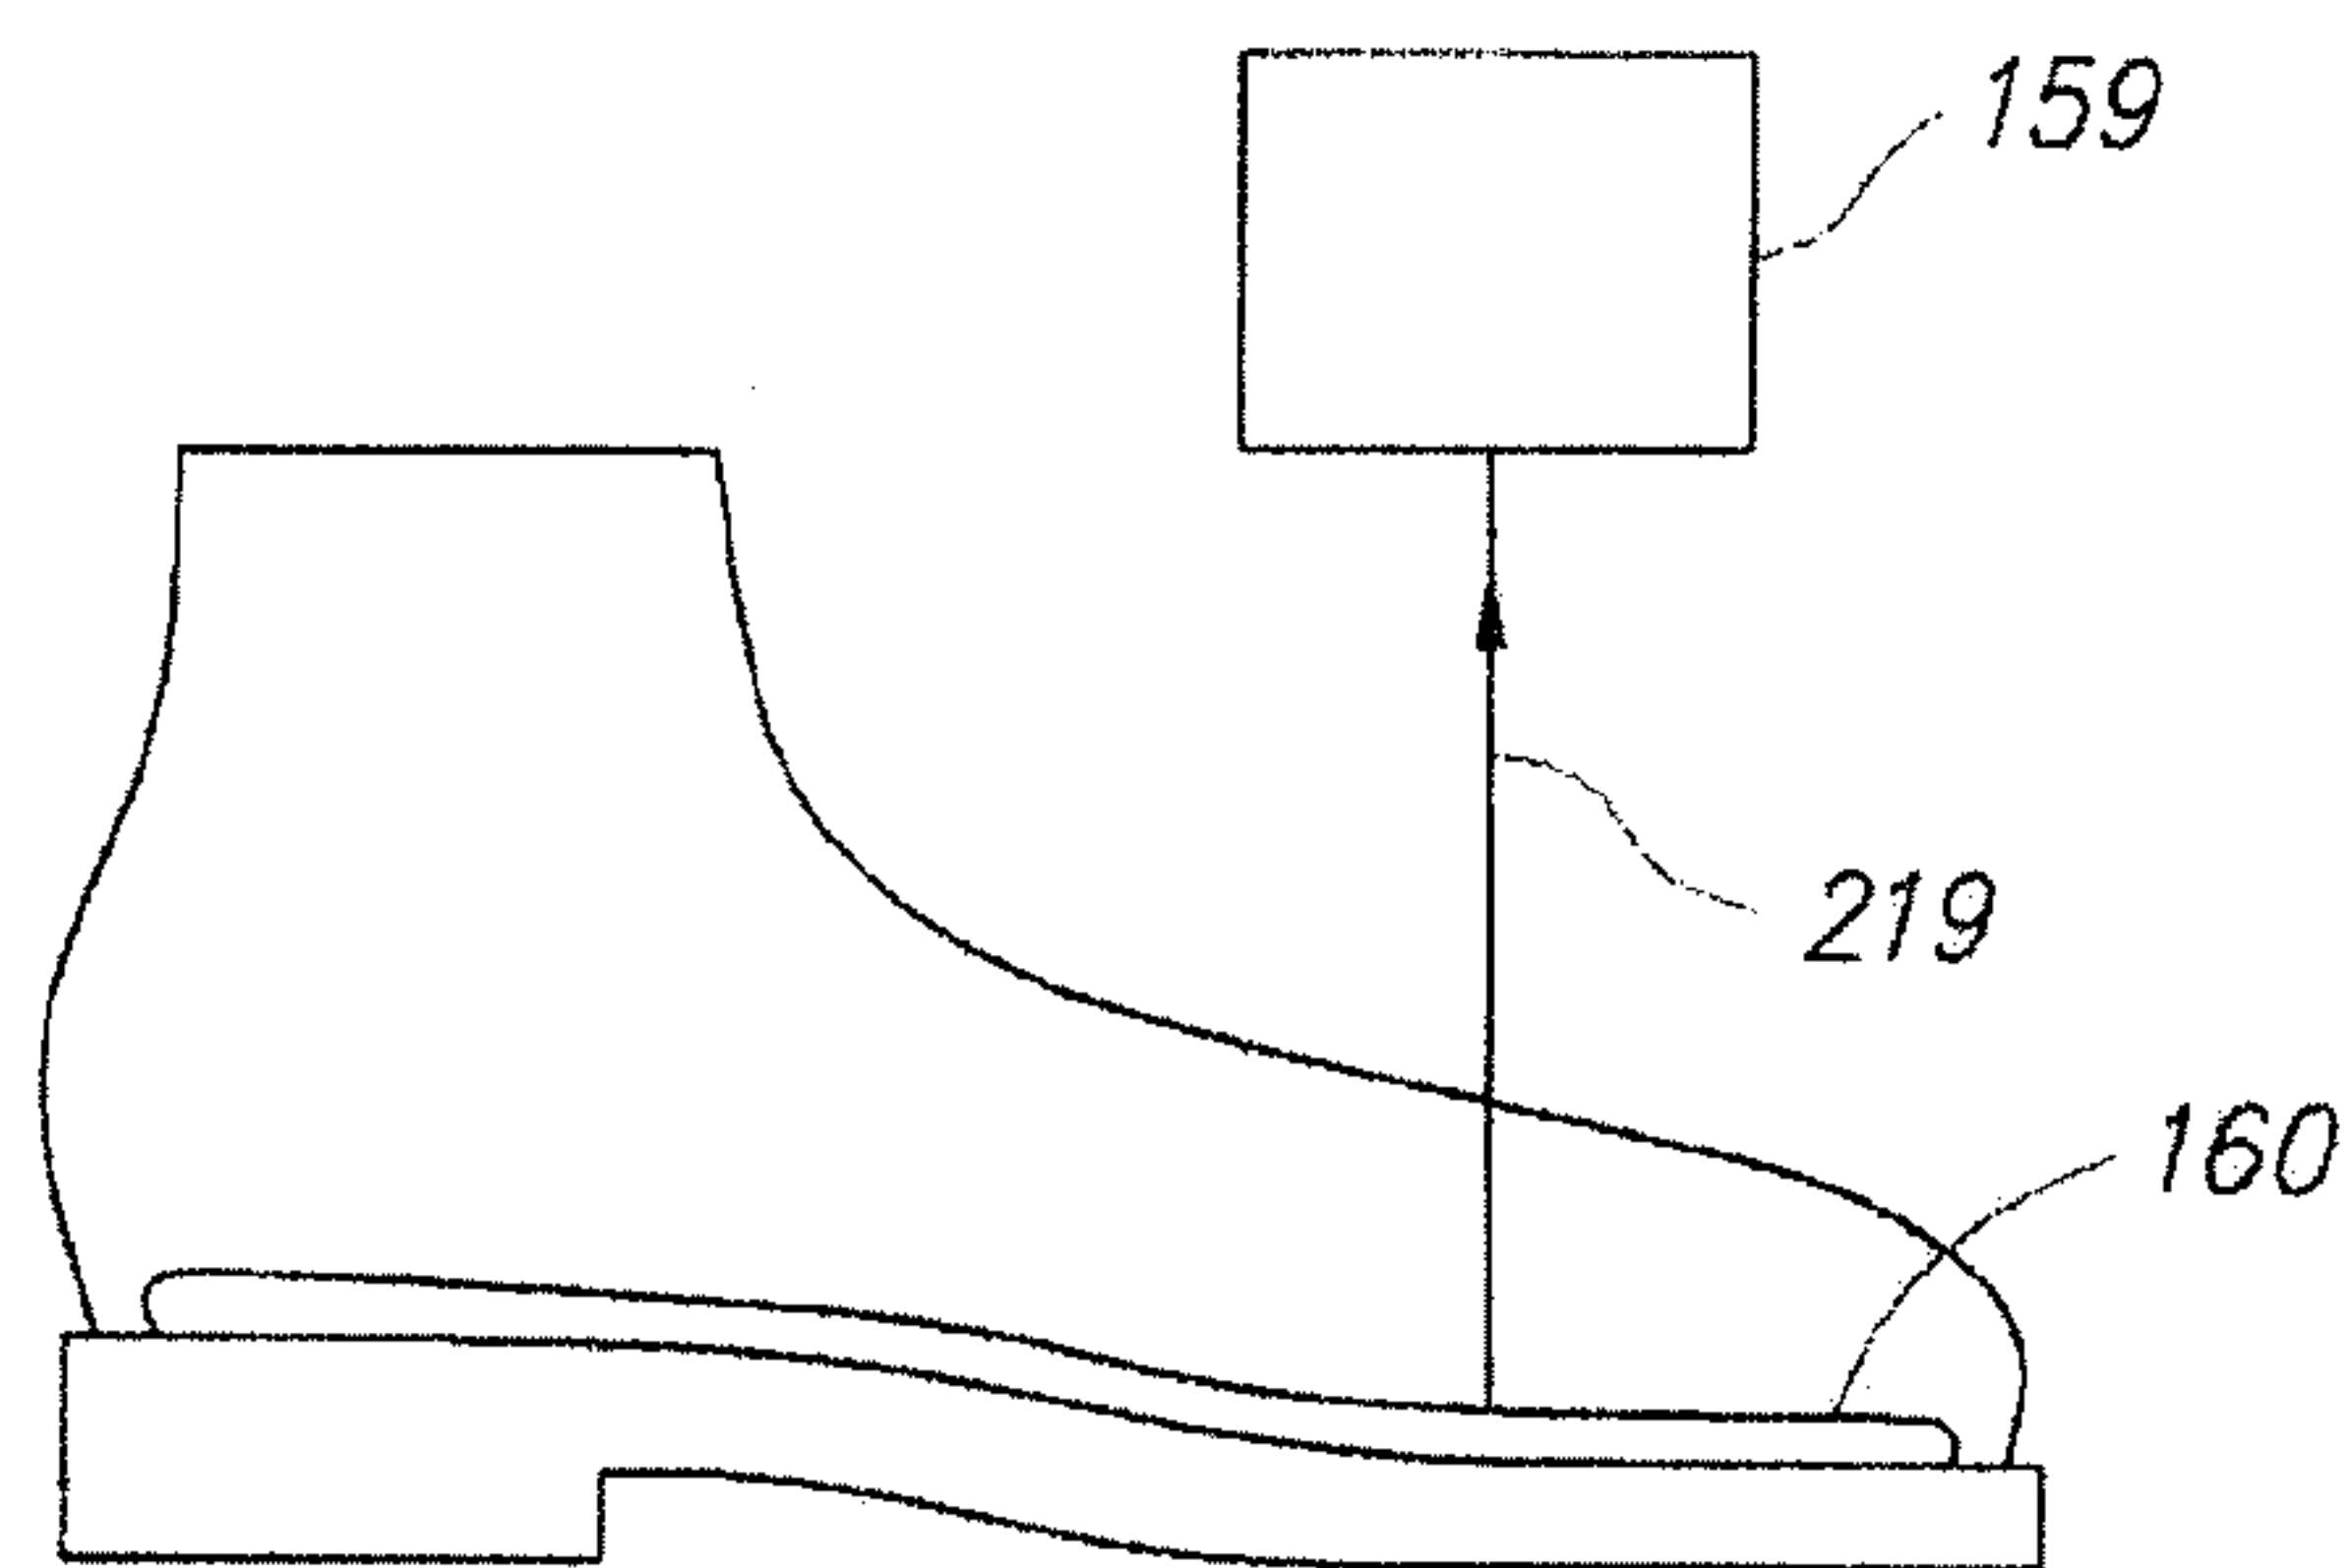


Fig. 30

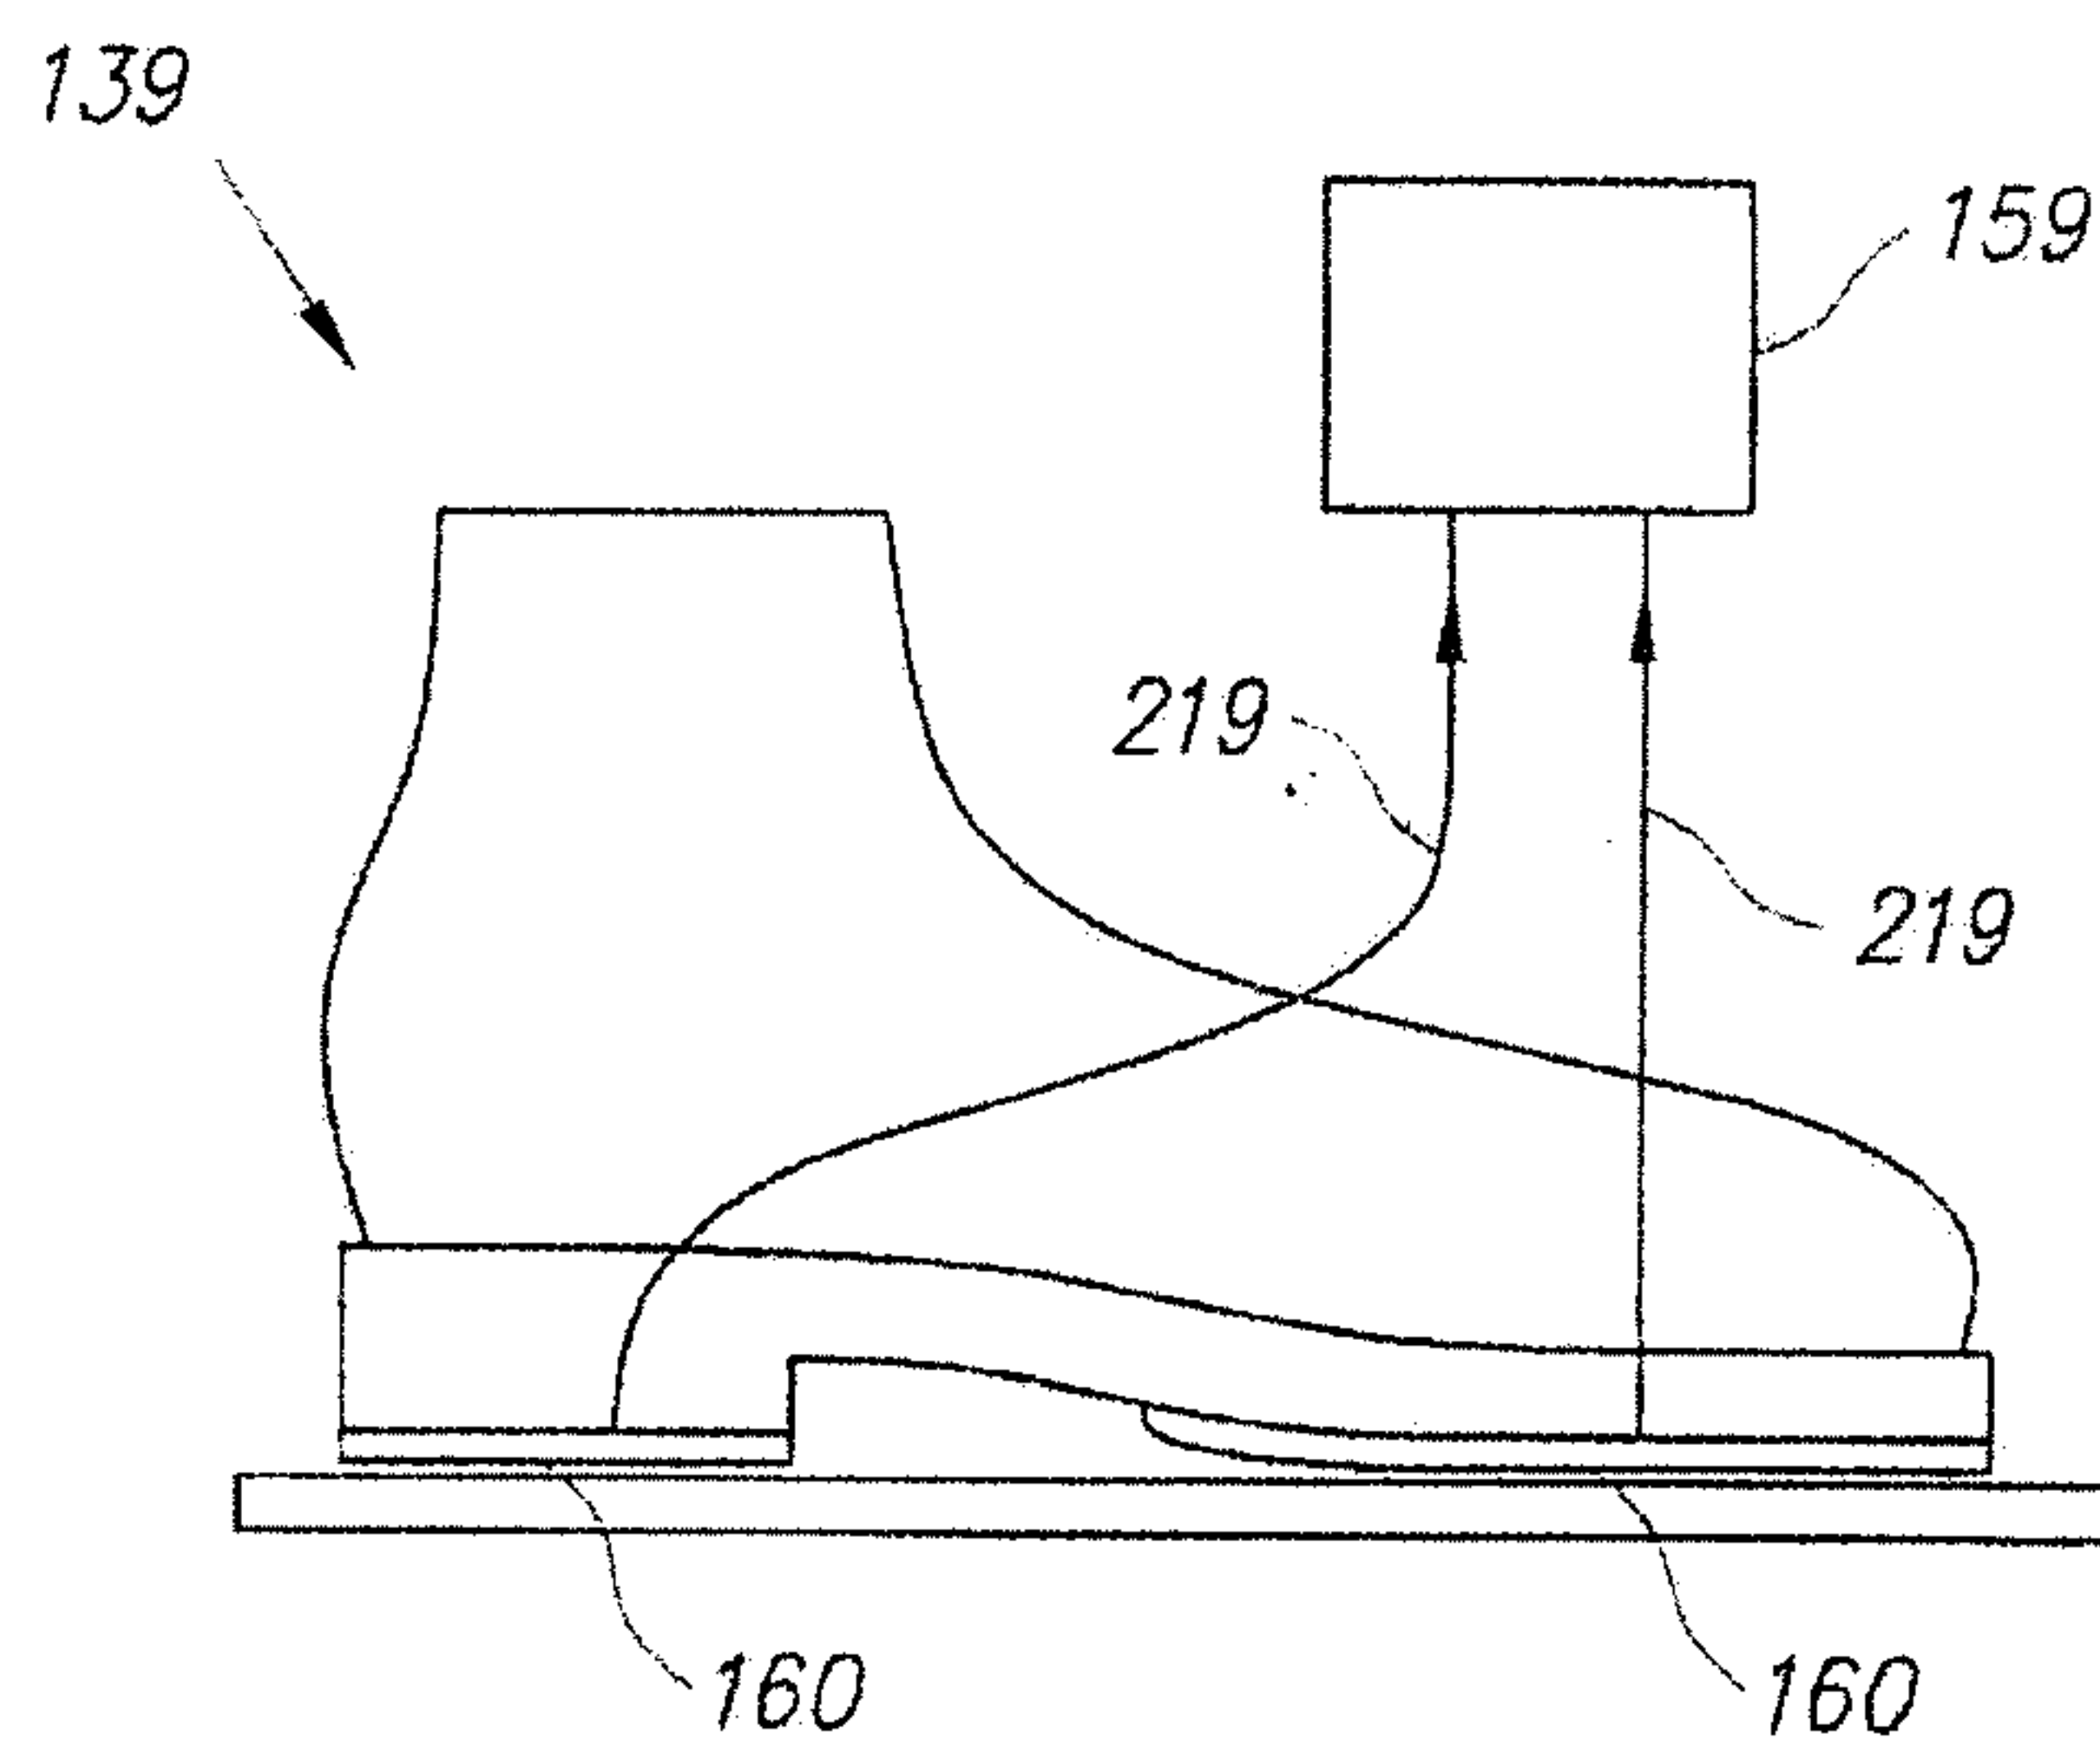


Fig. 31

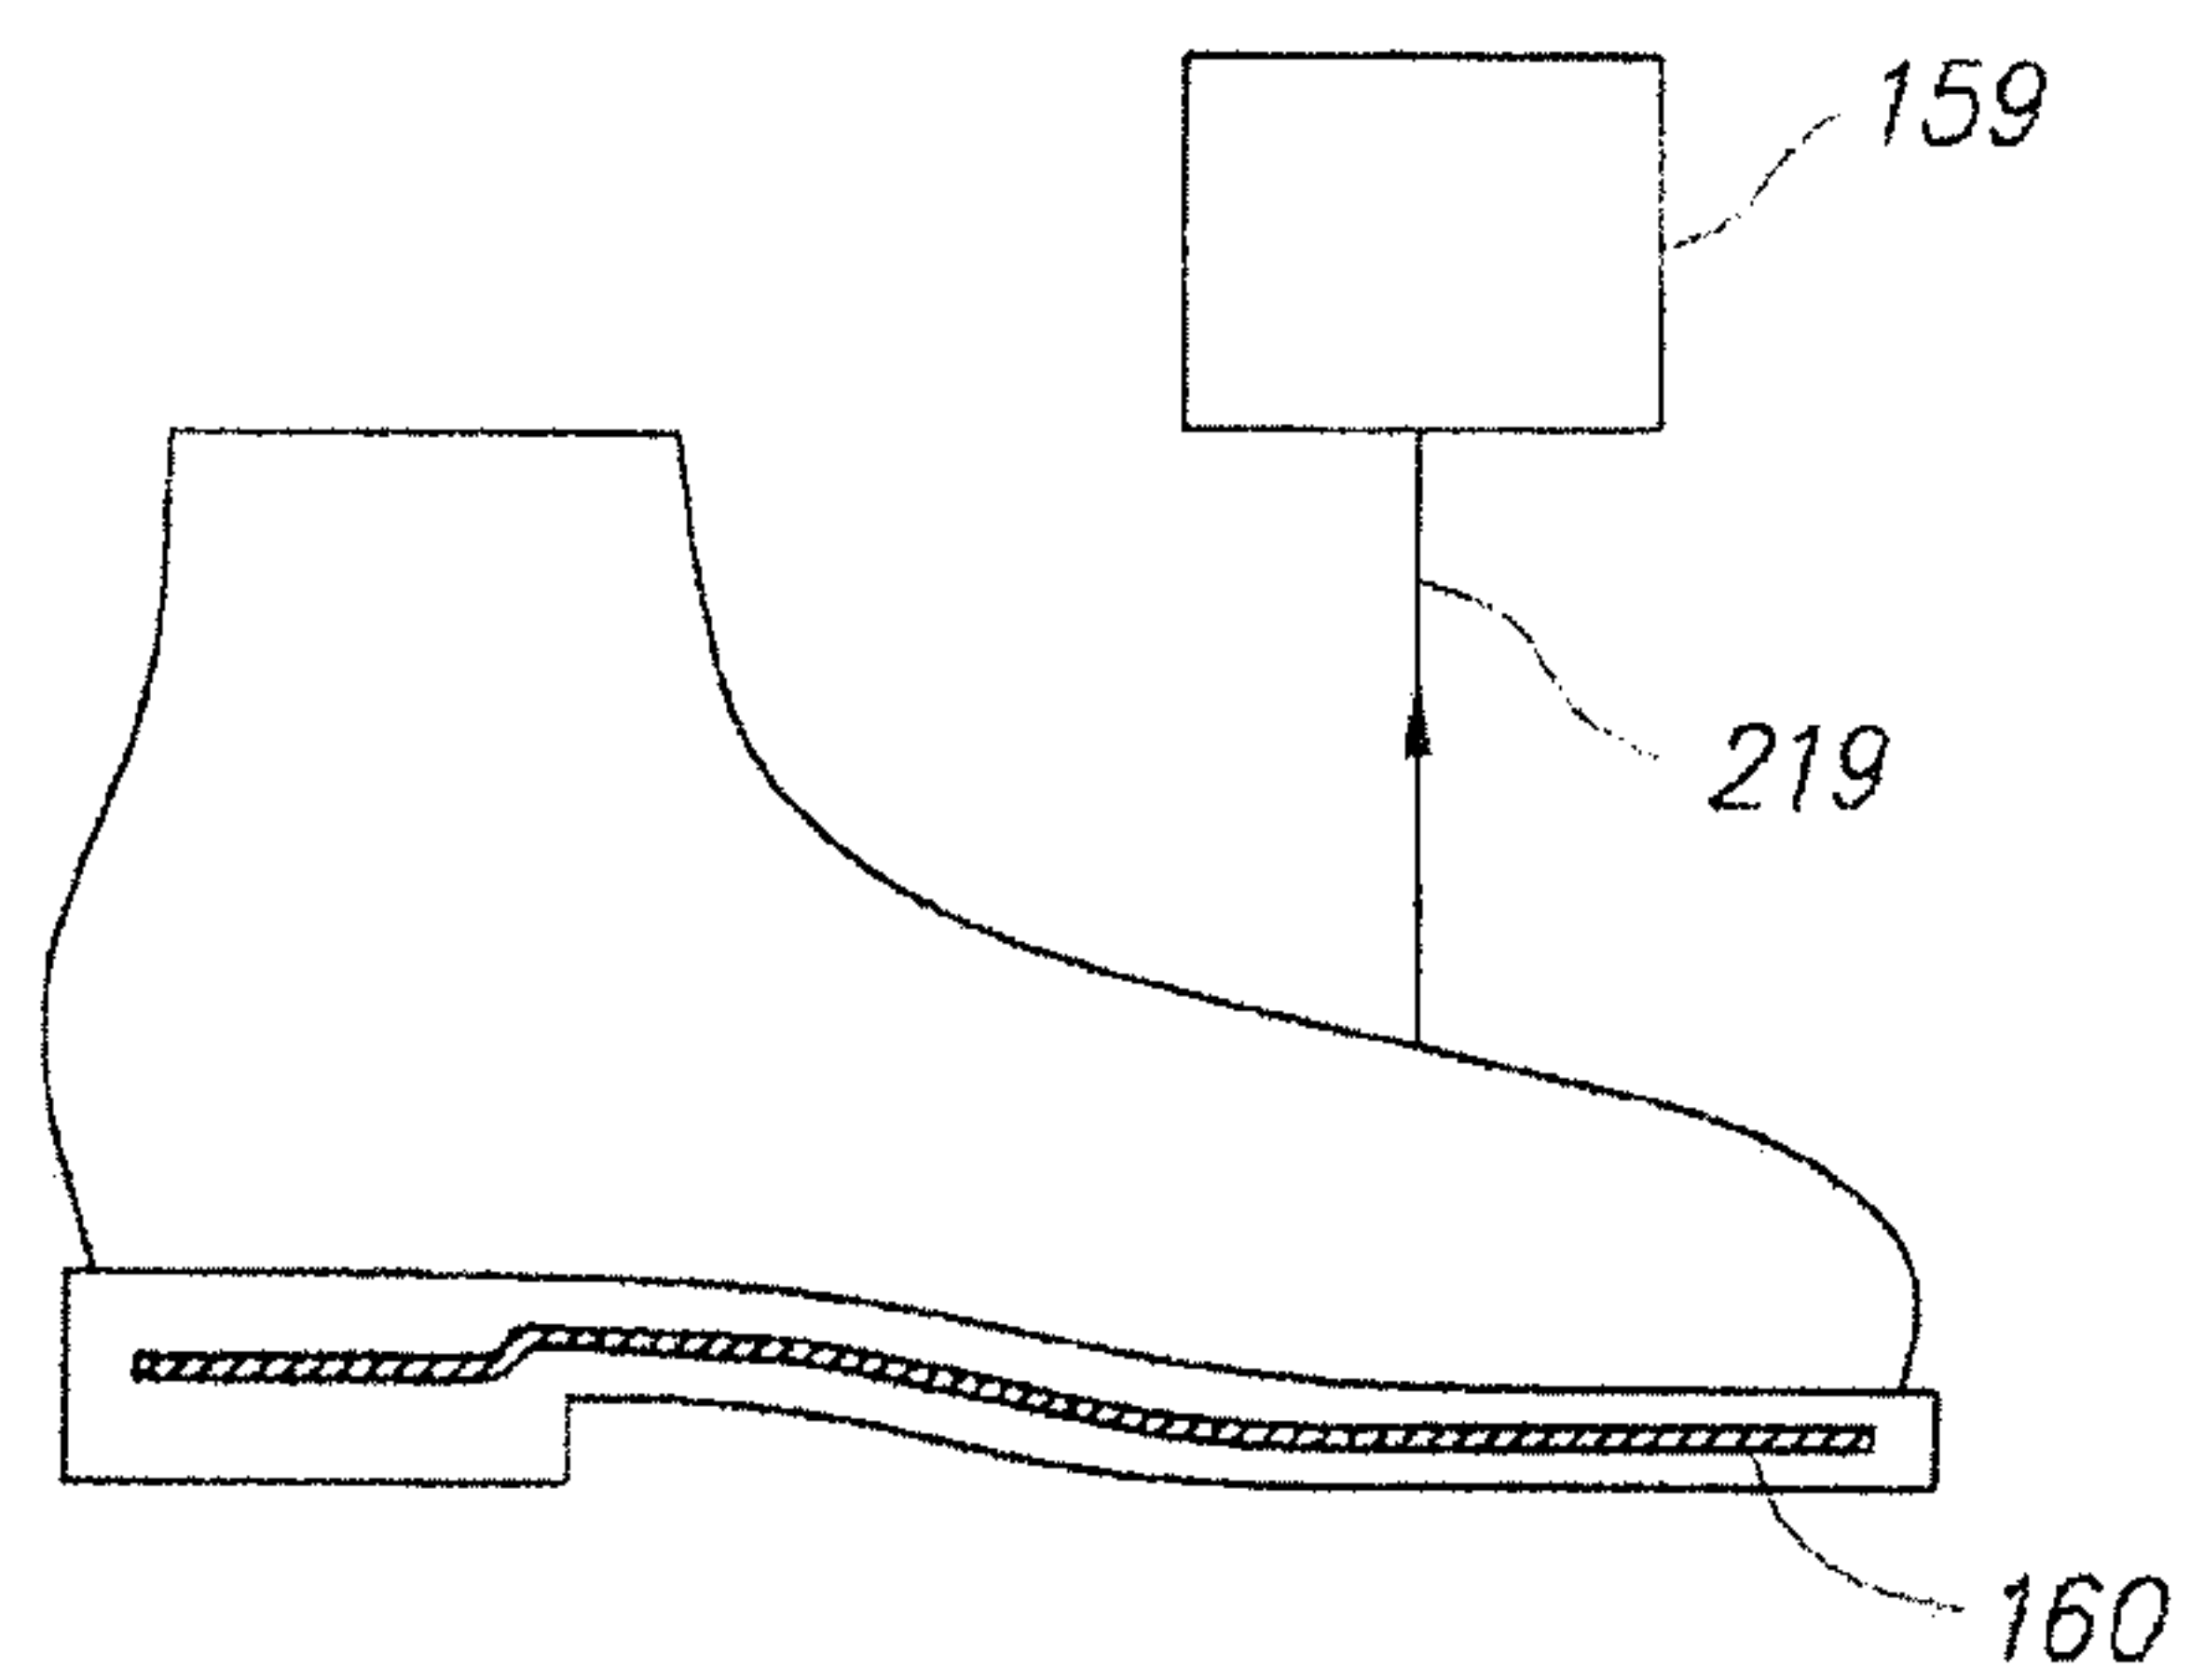


Fig. 32

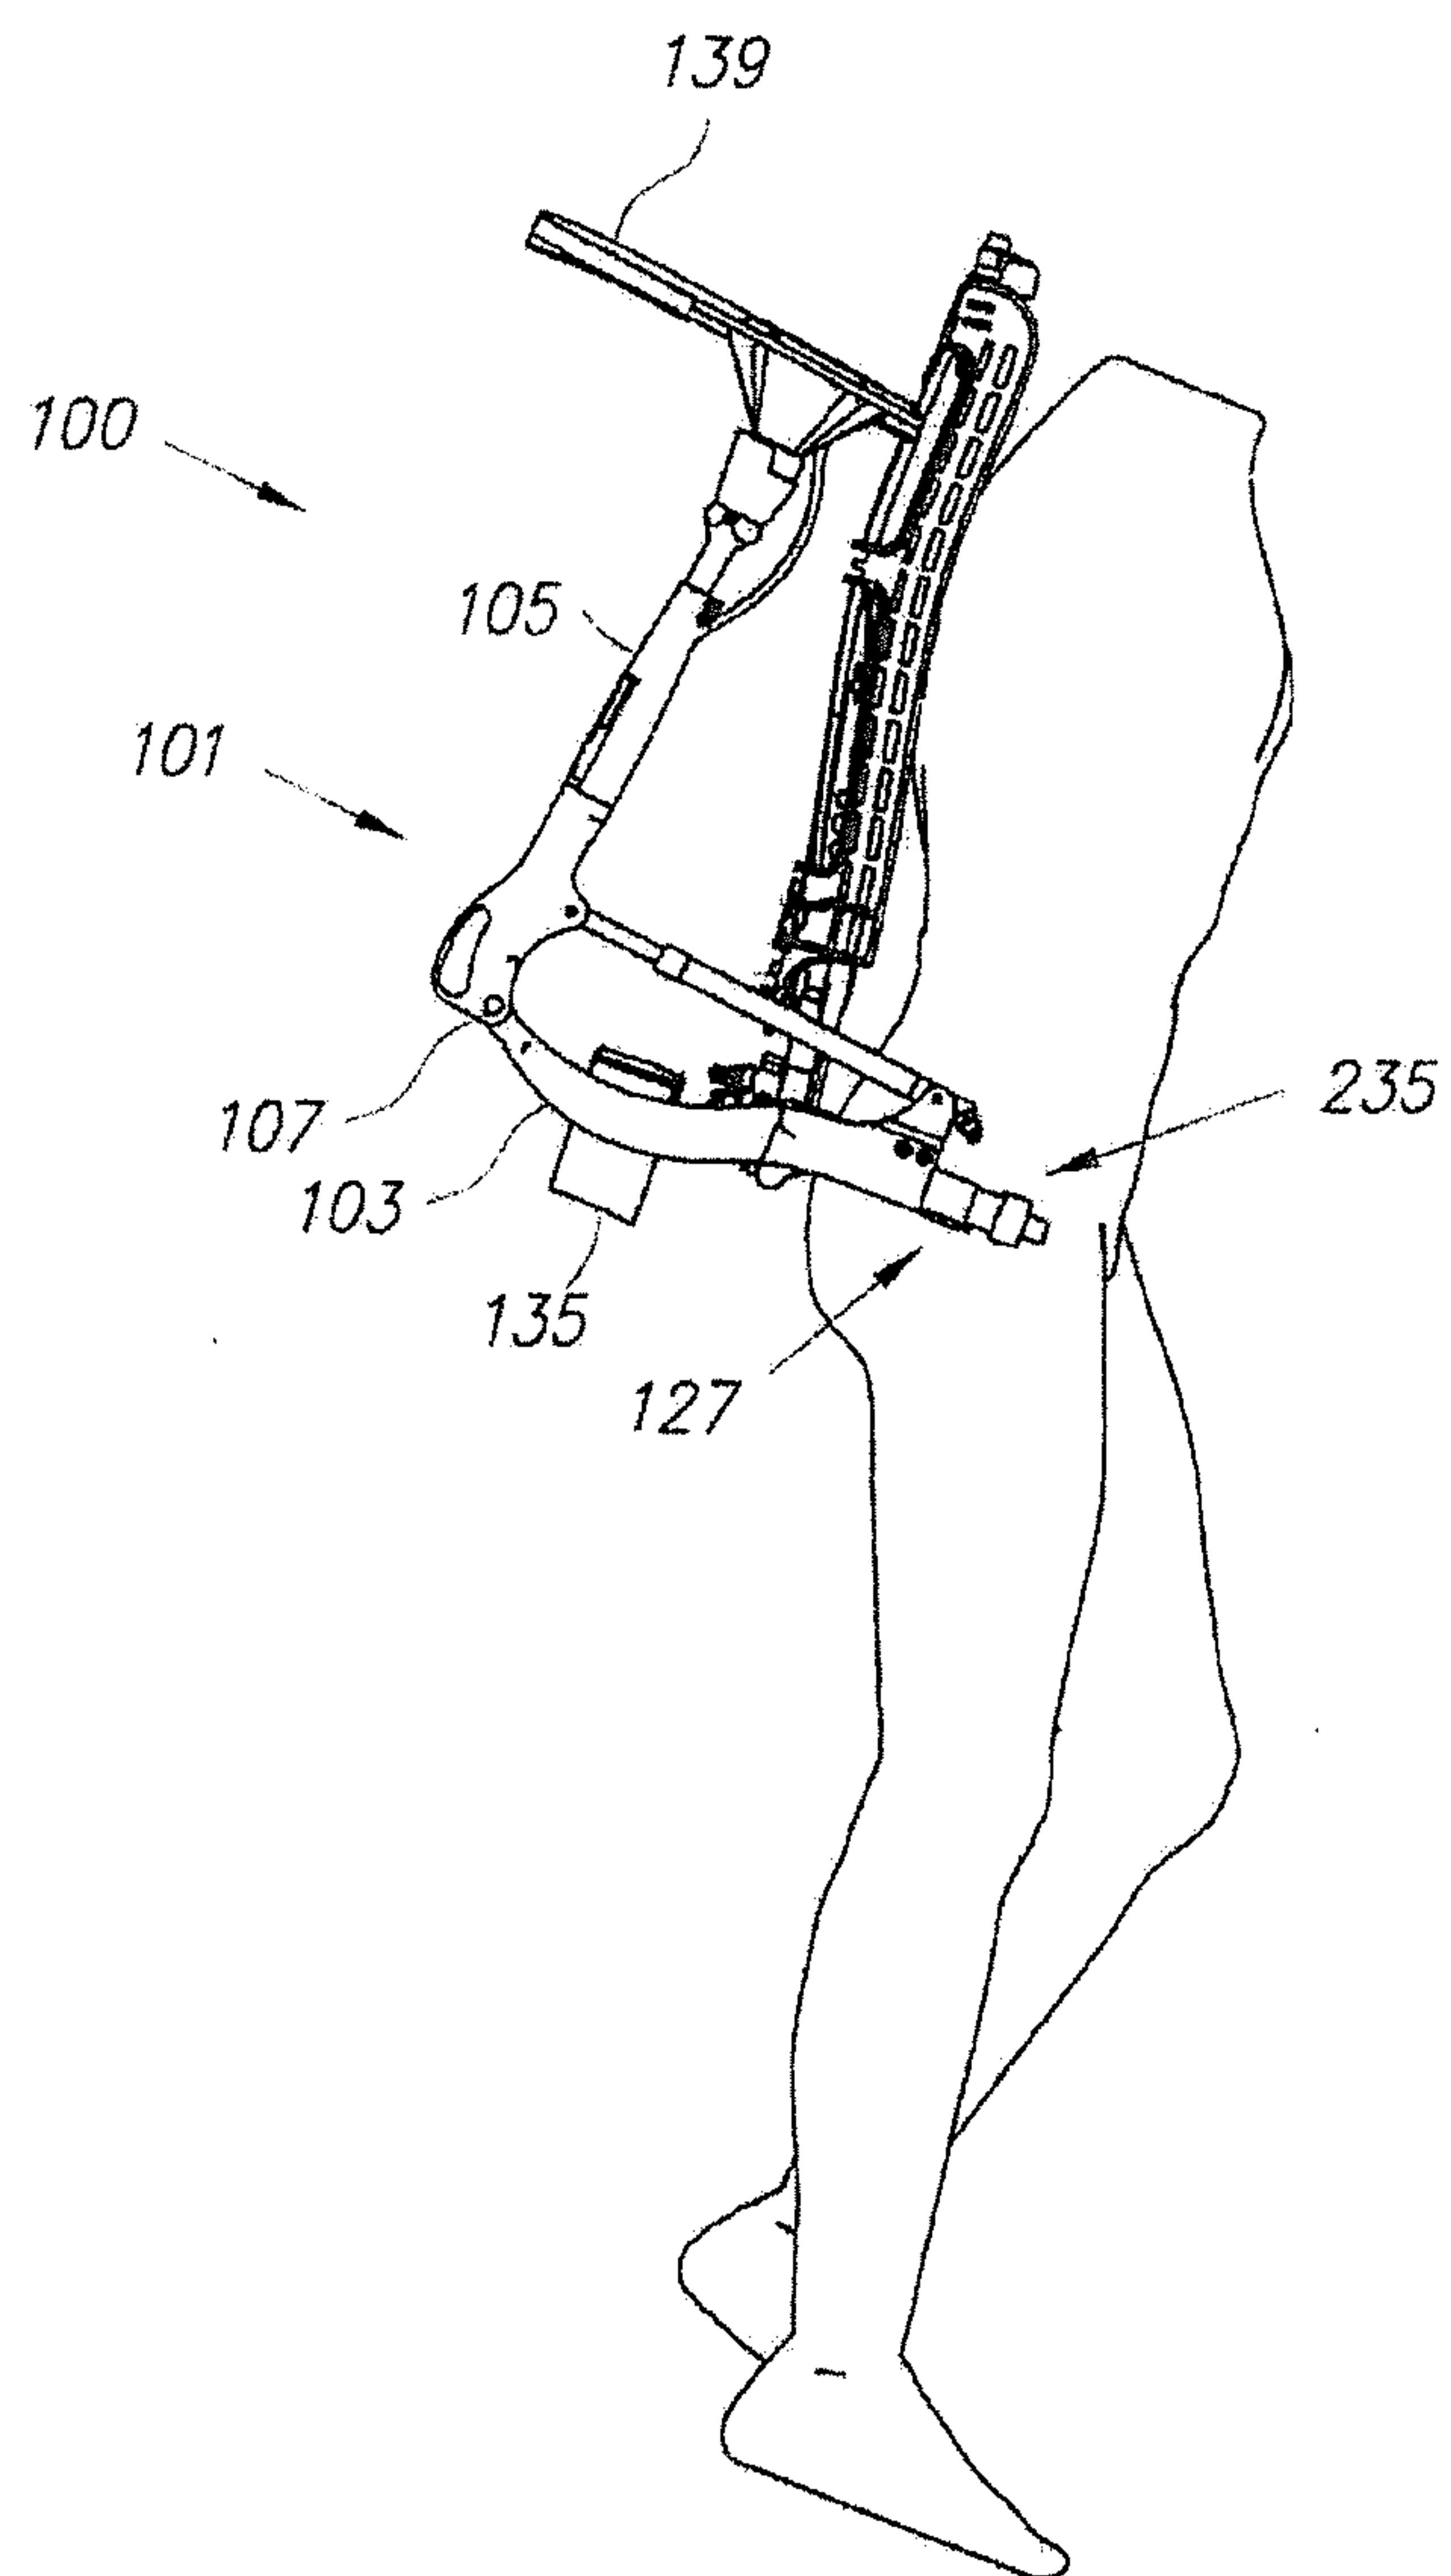


Fig. 33

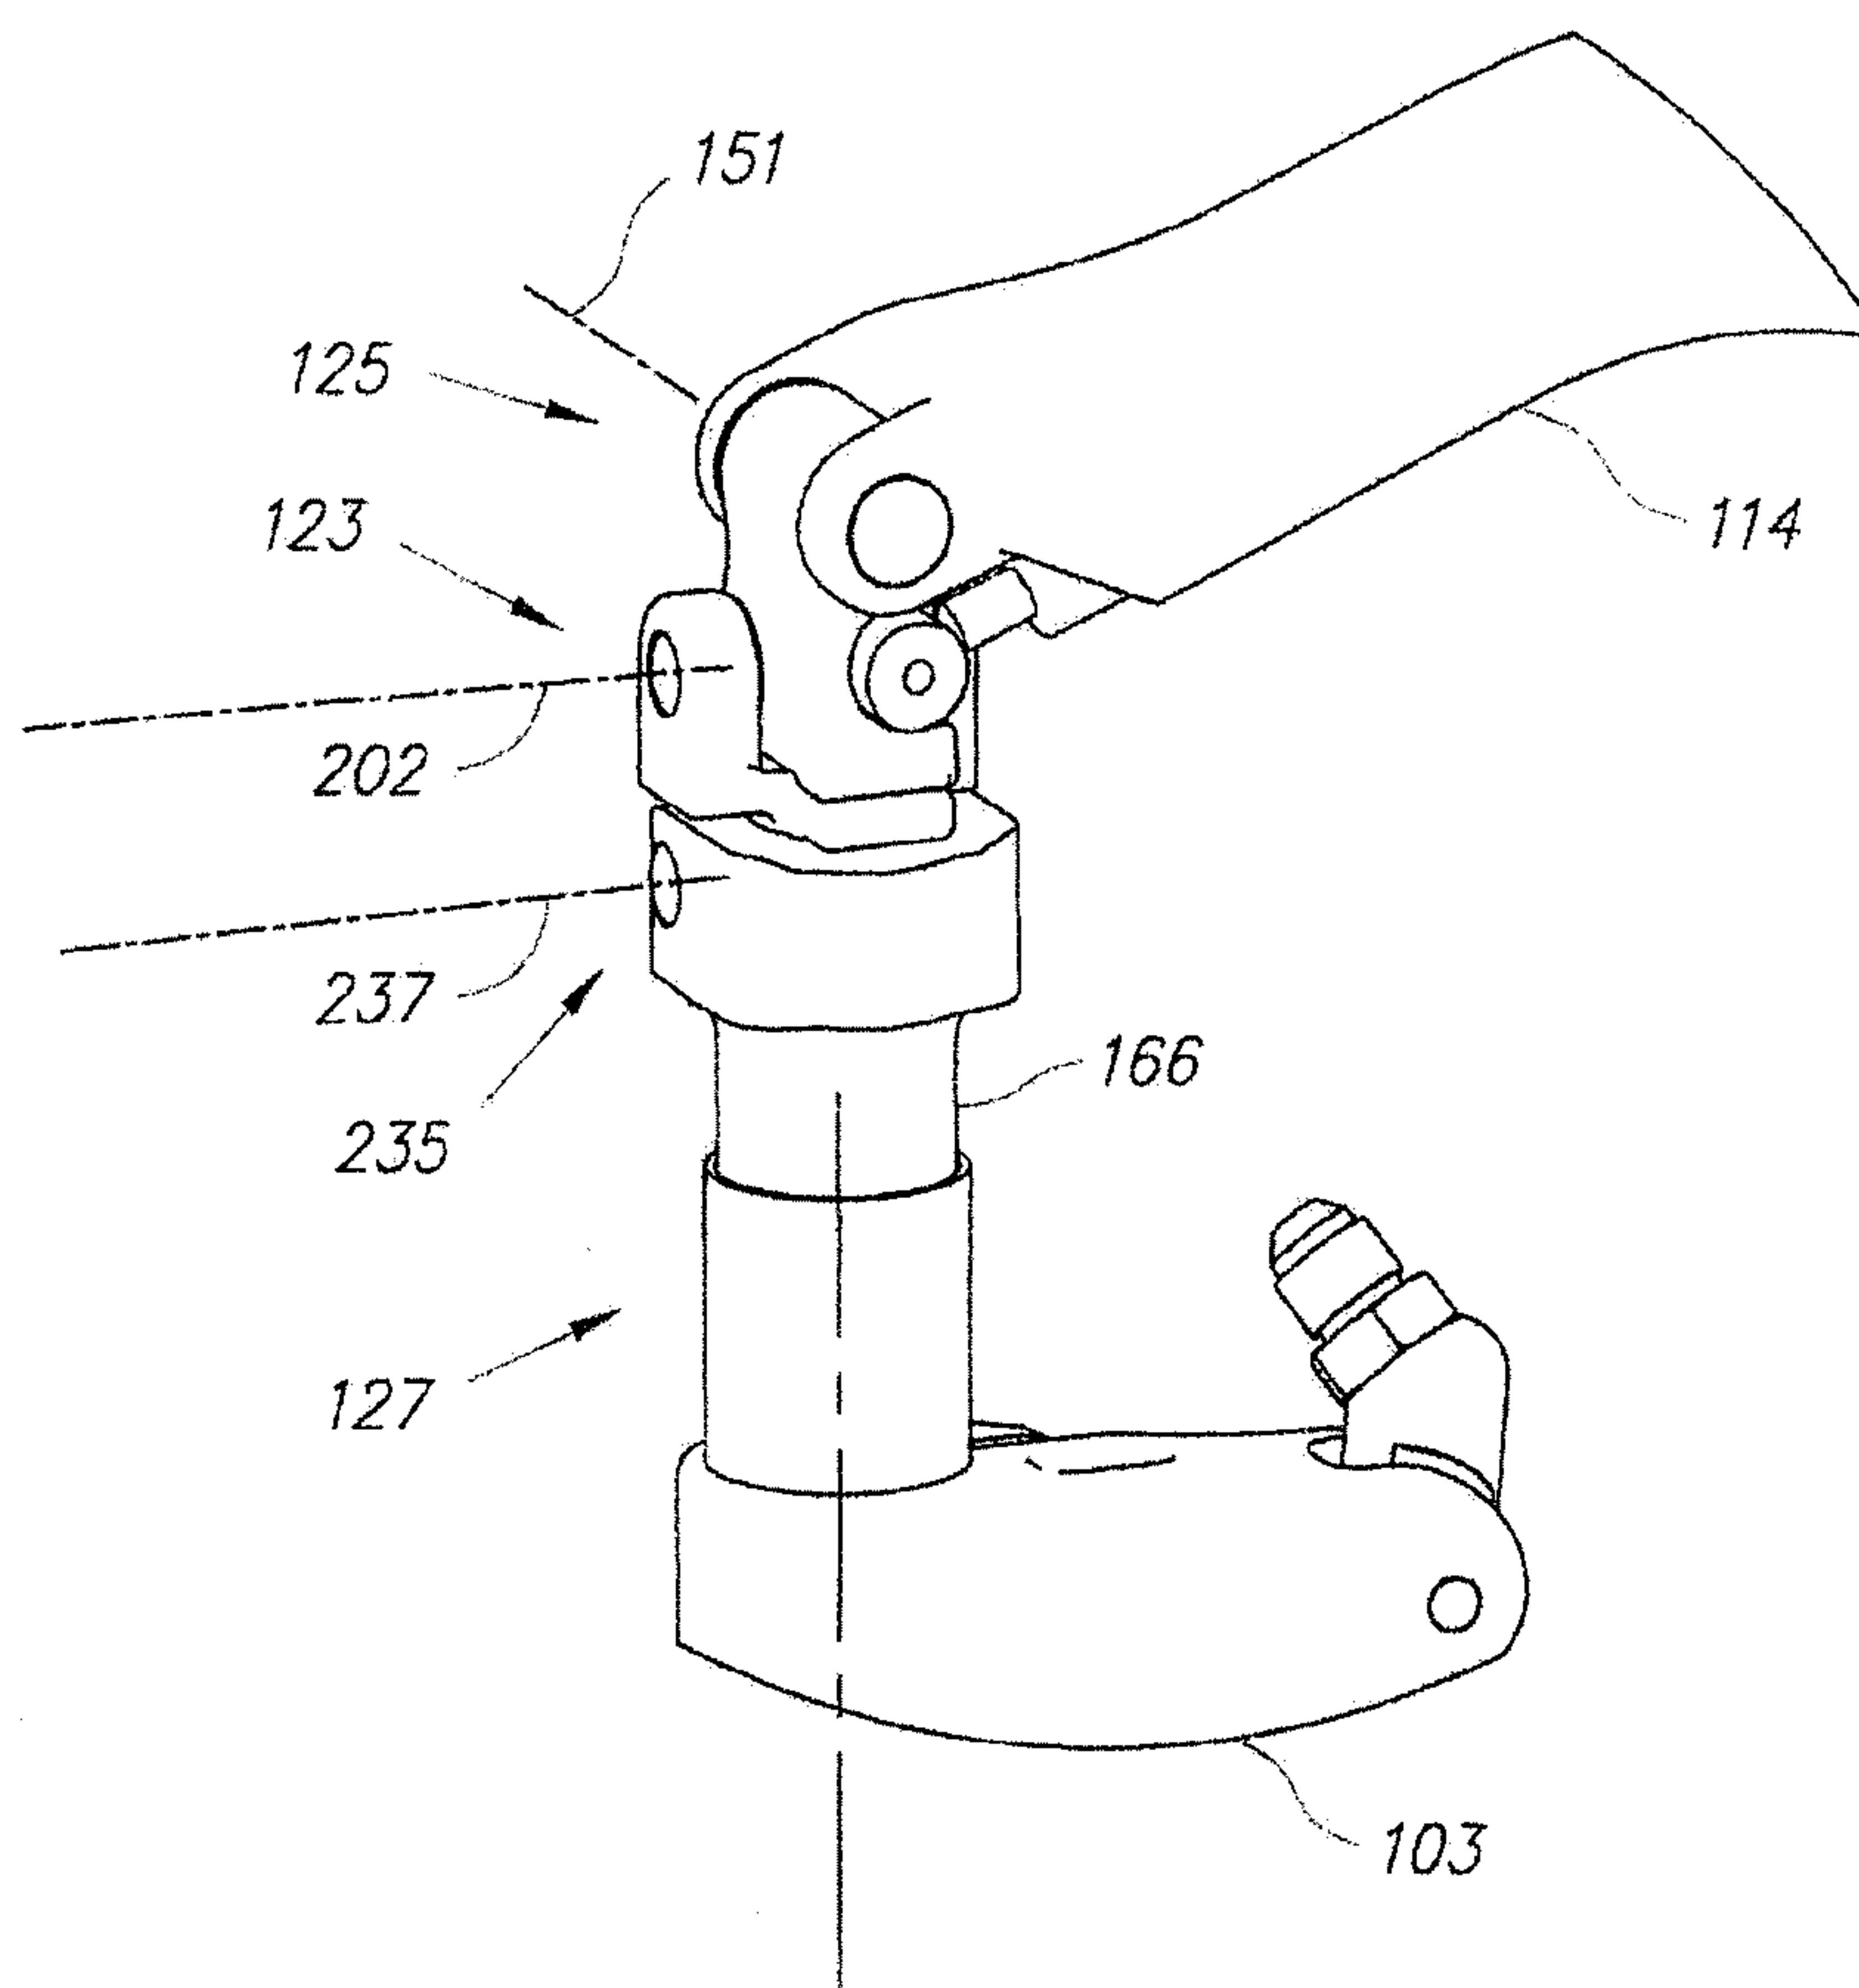


Fig. 34

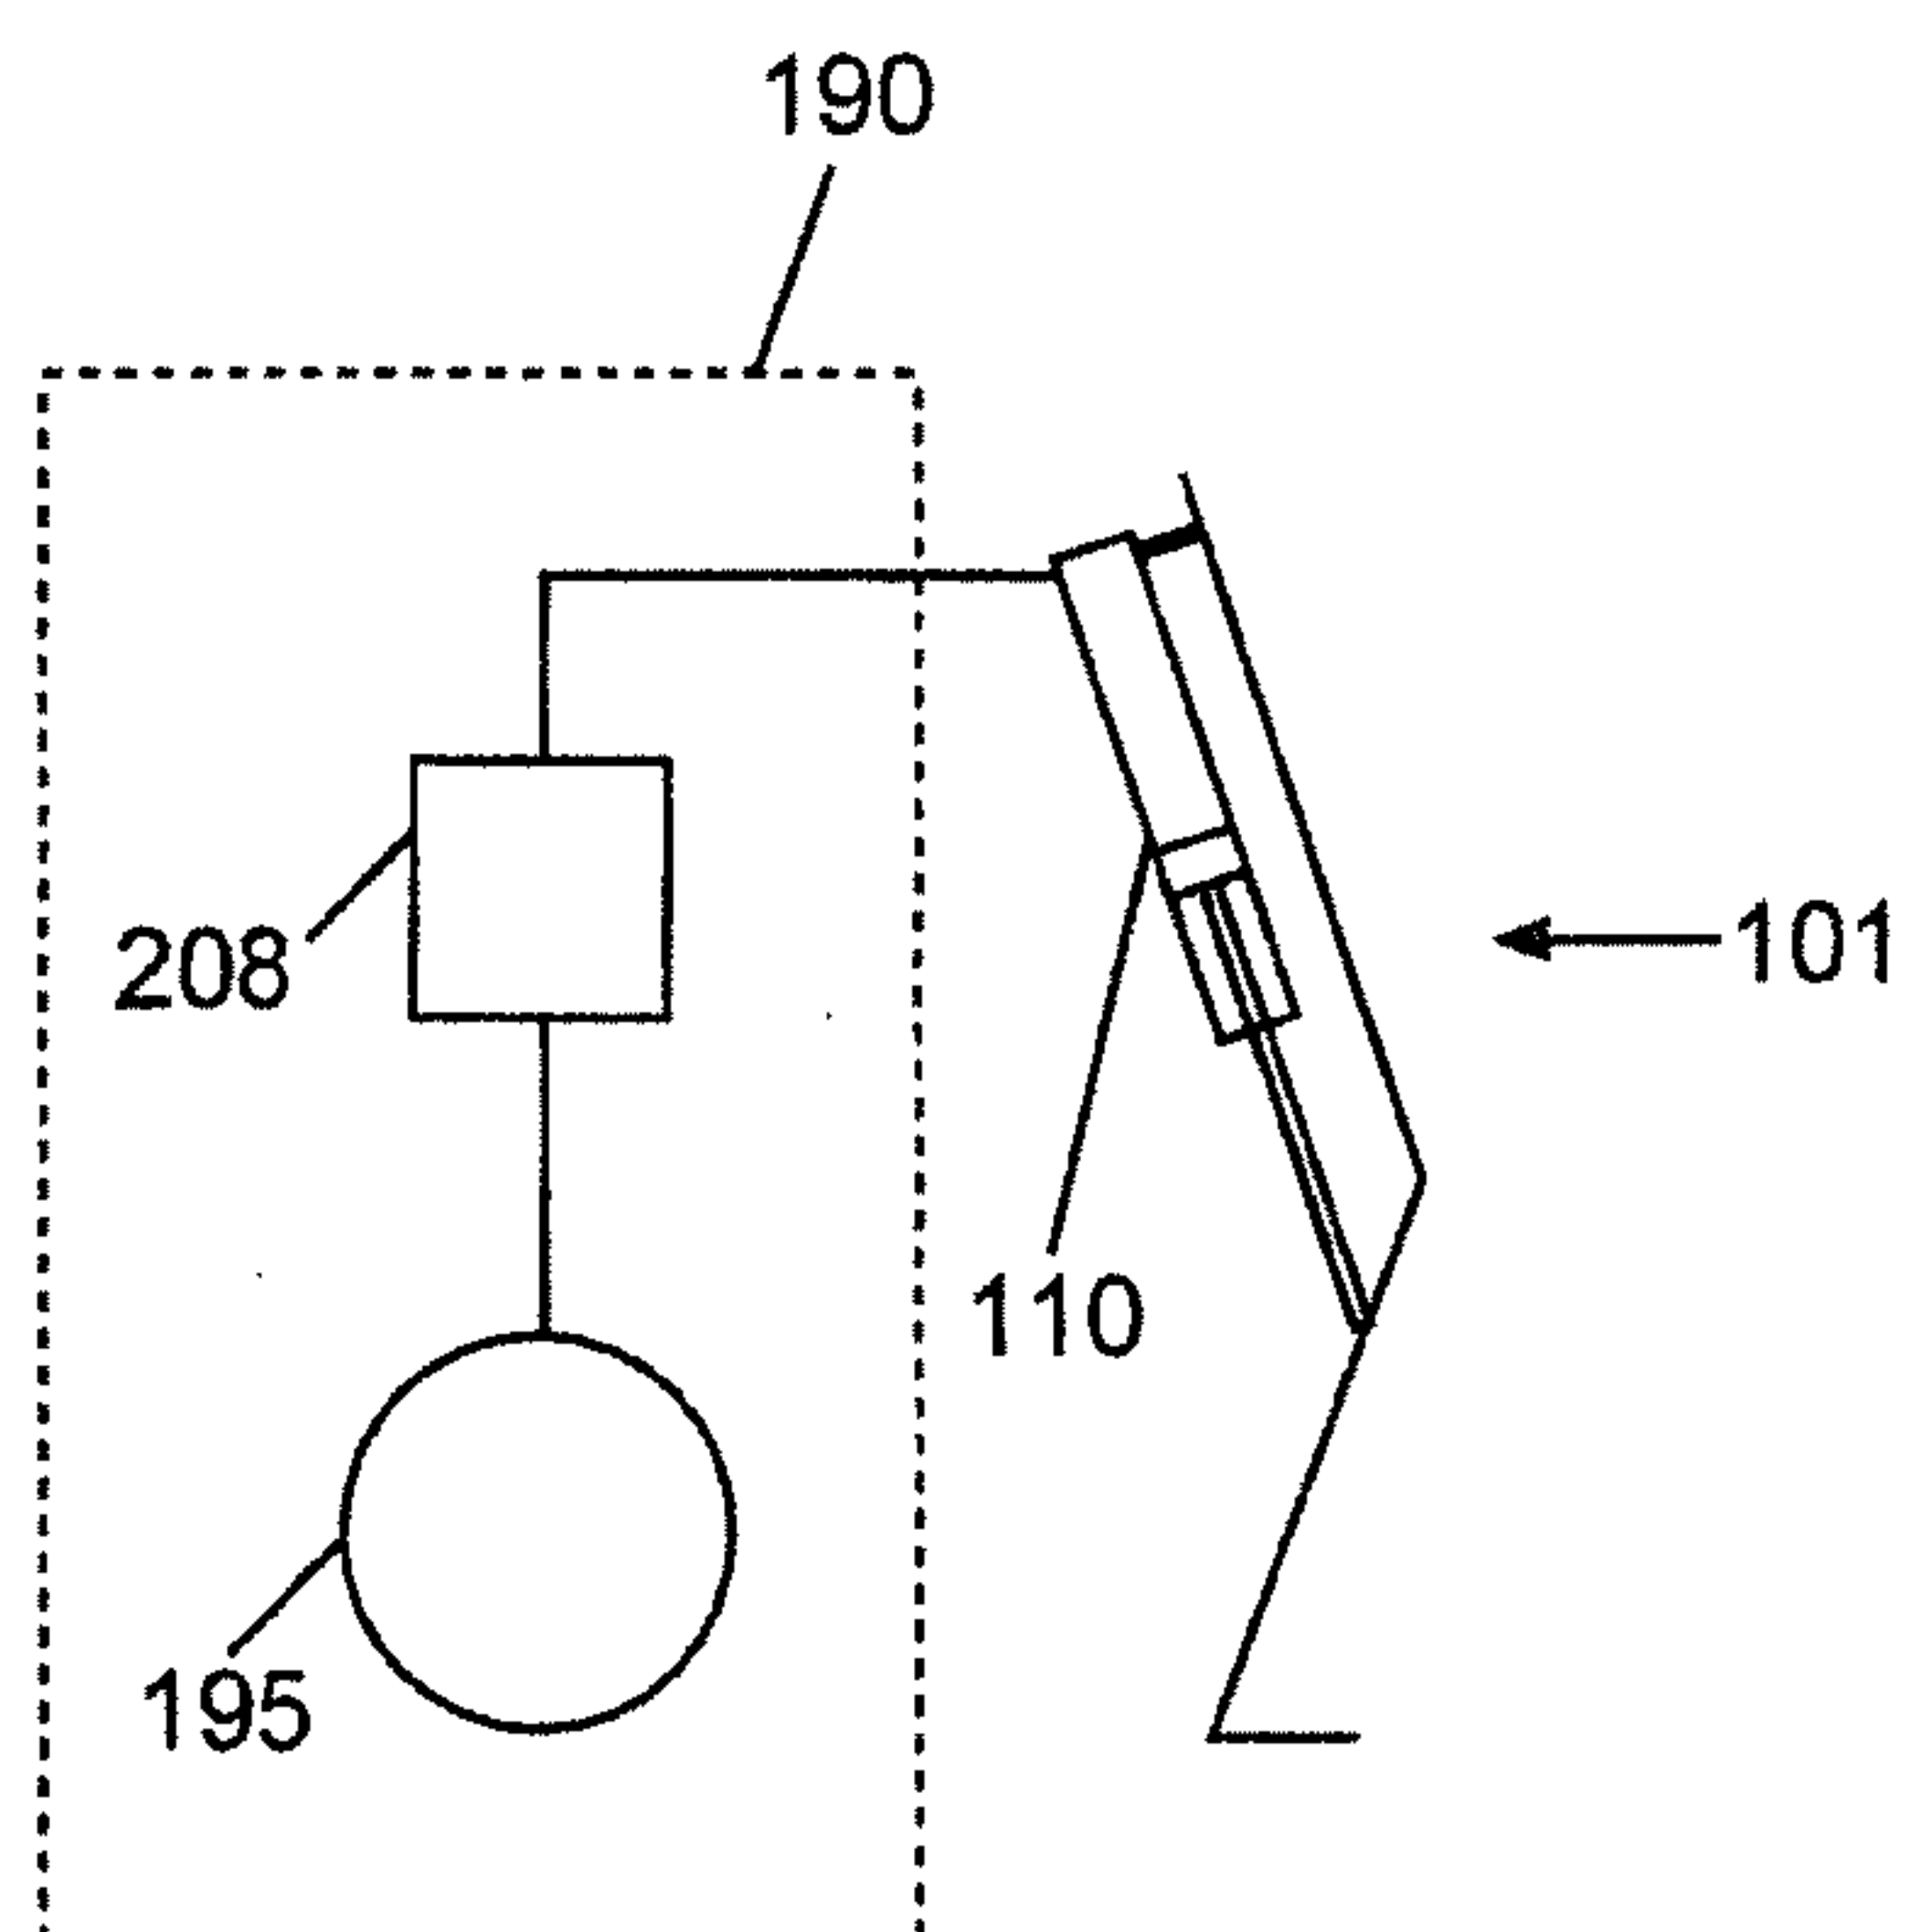


Figure 36

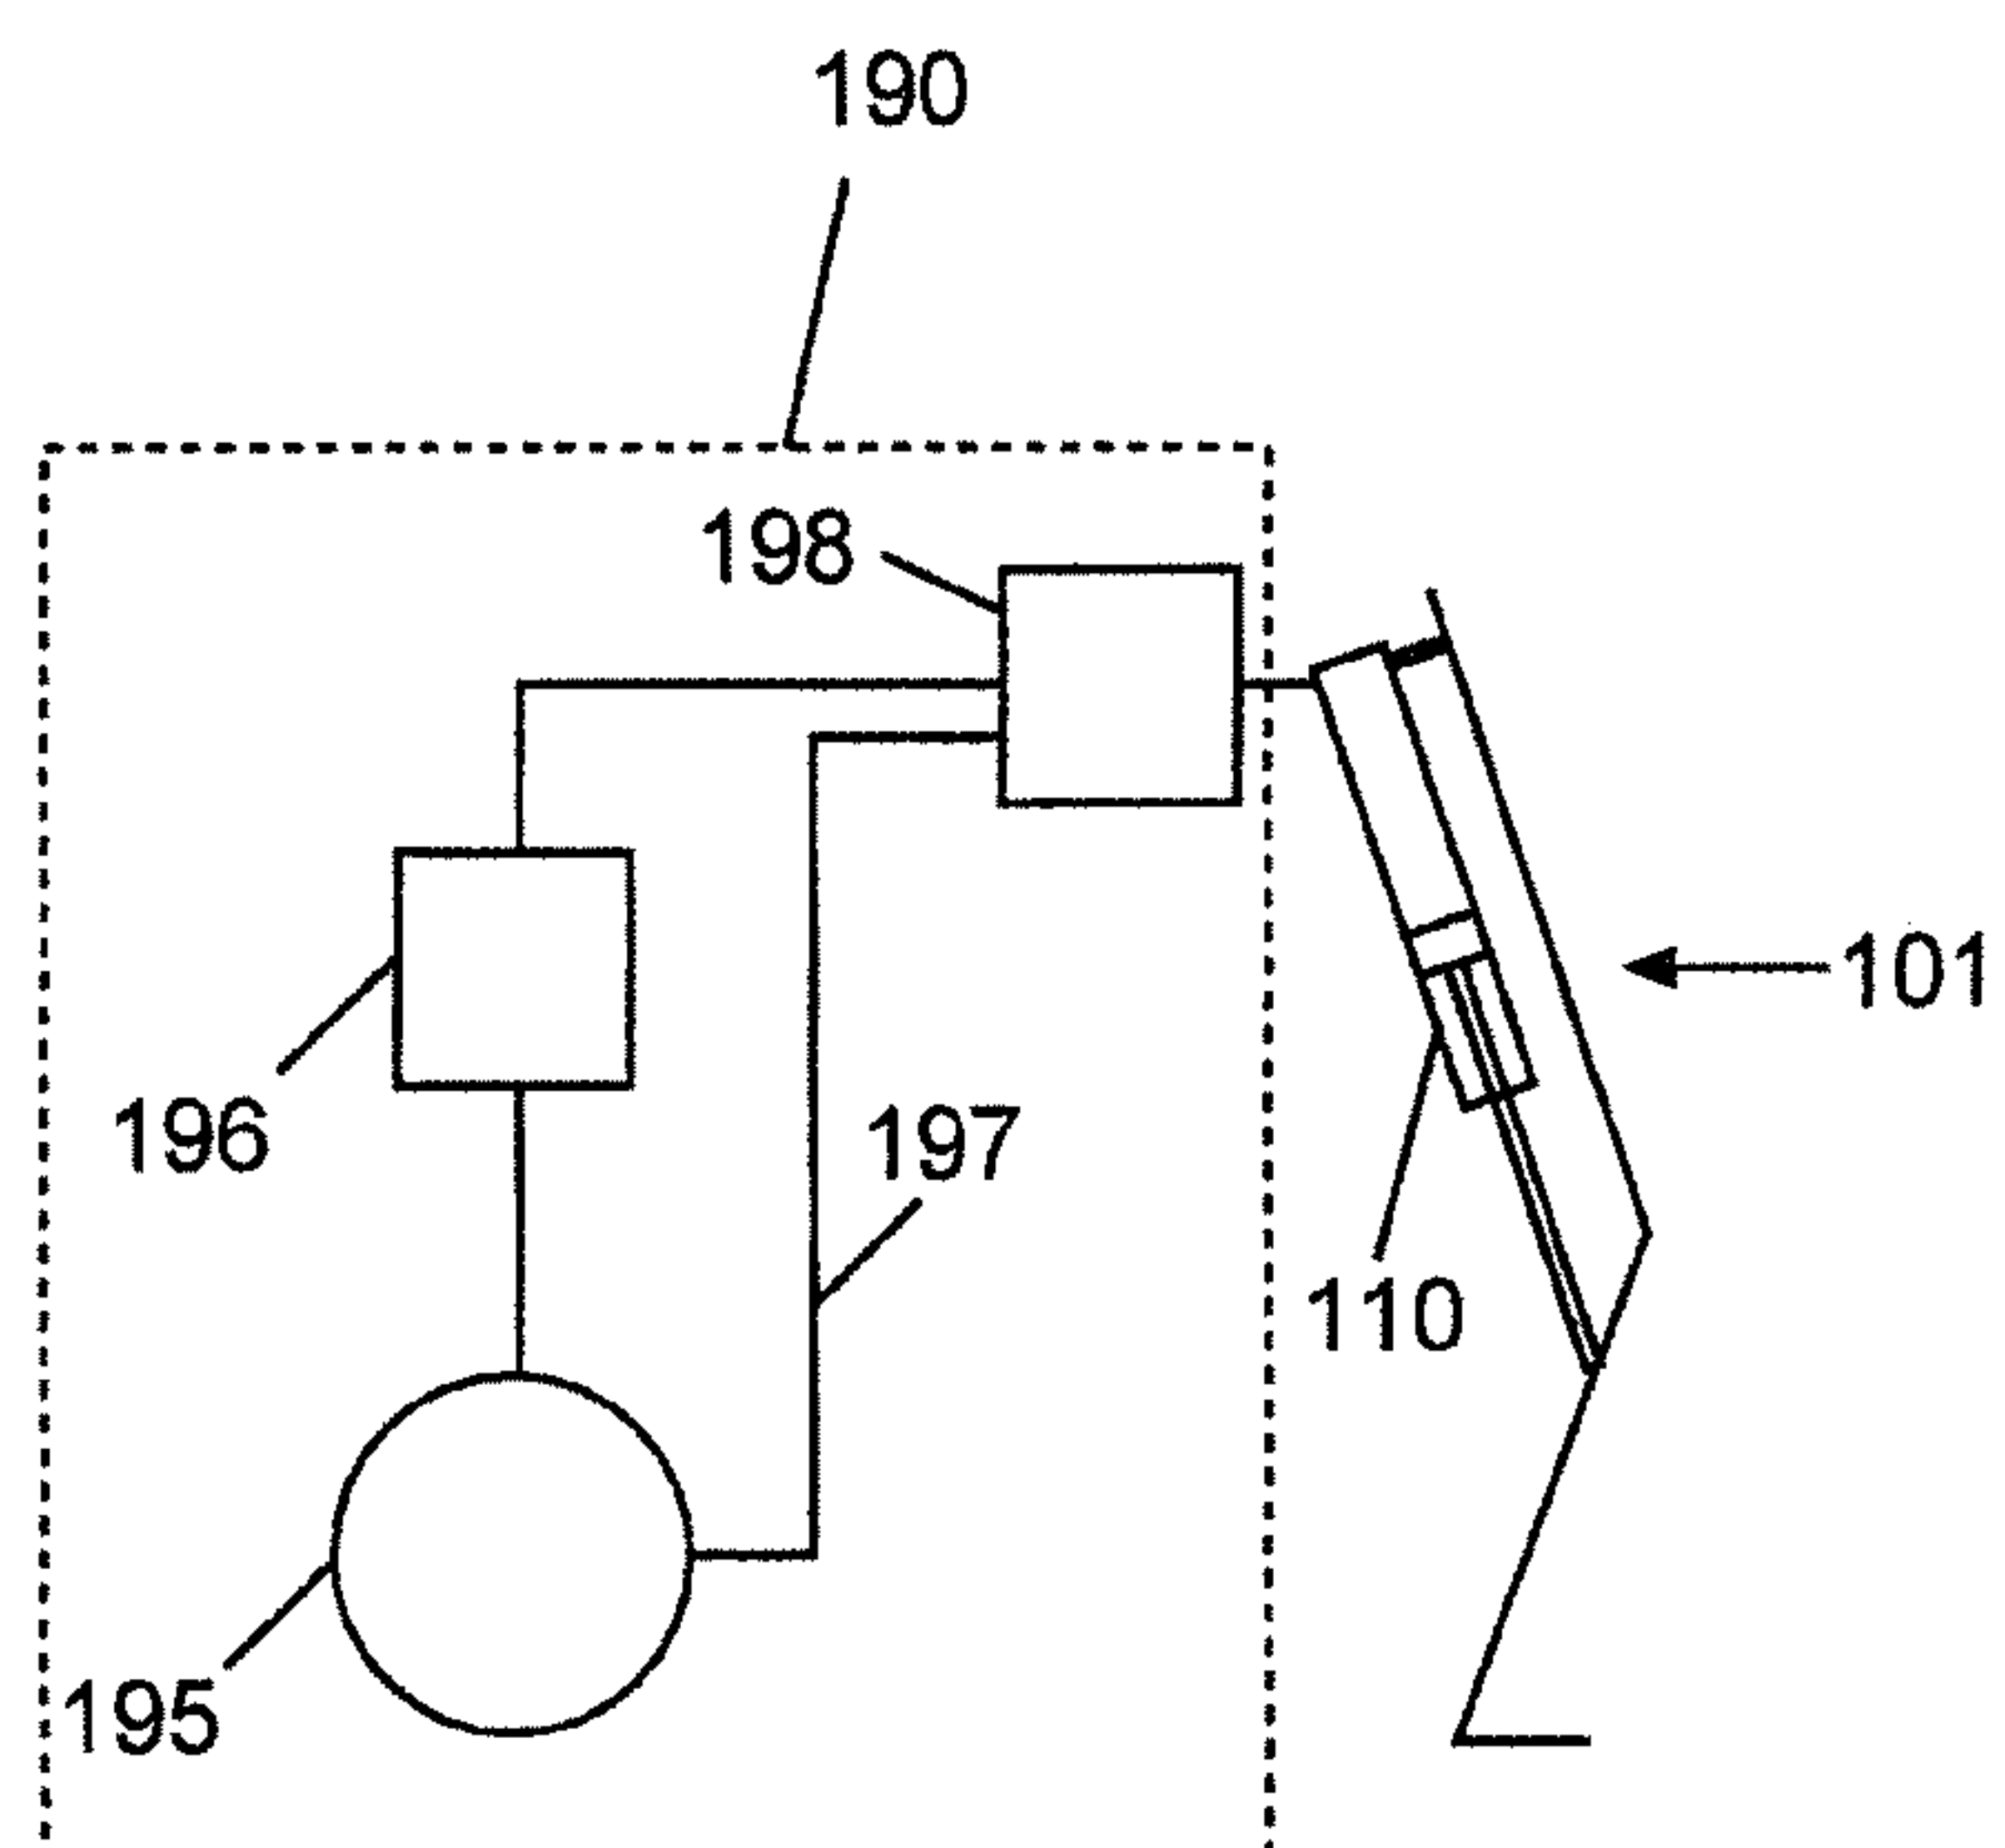


Figure 37

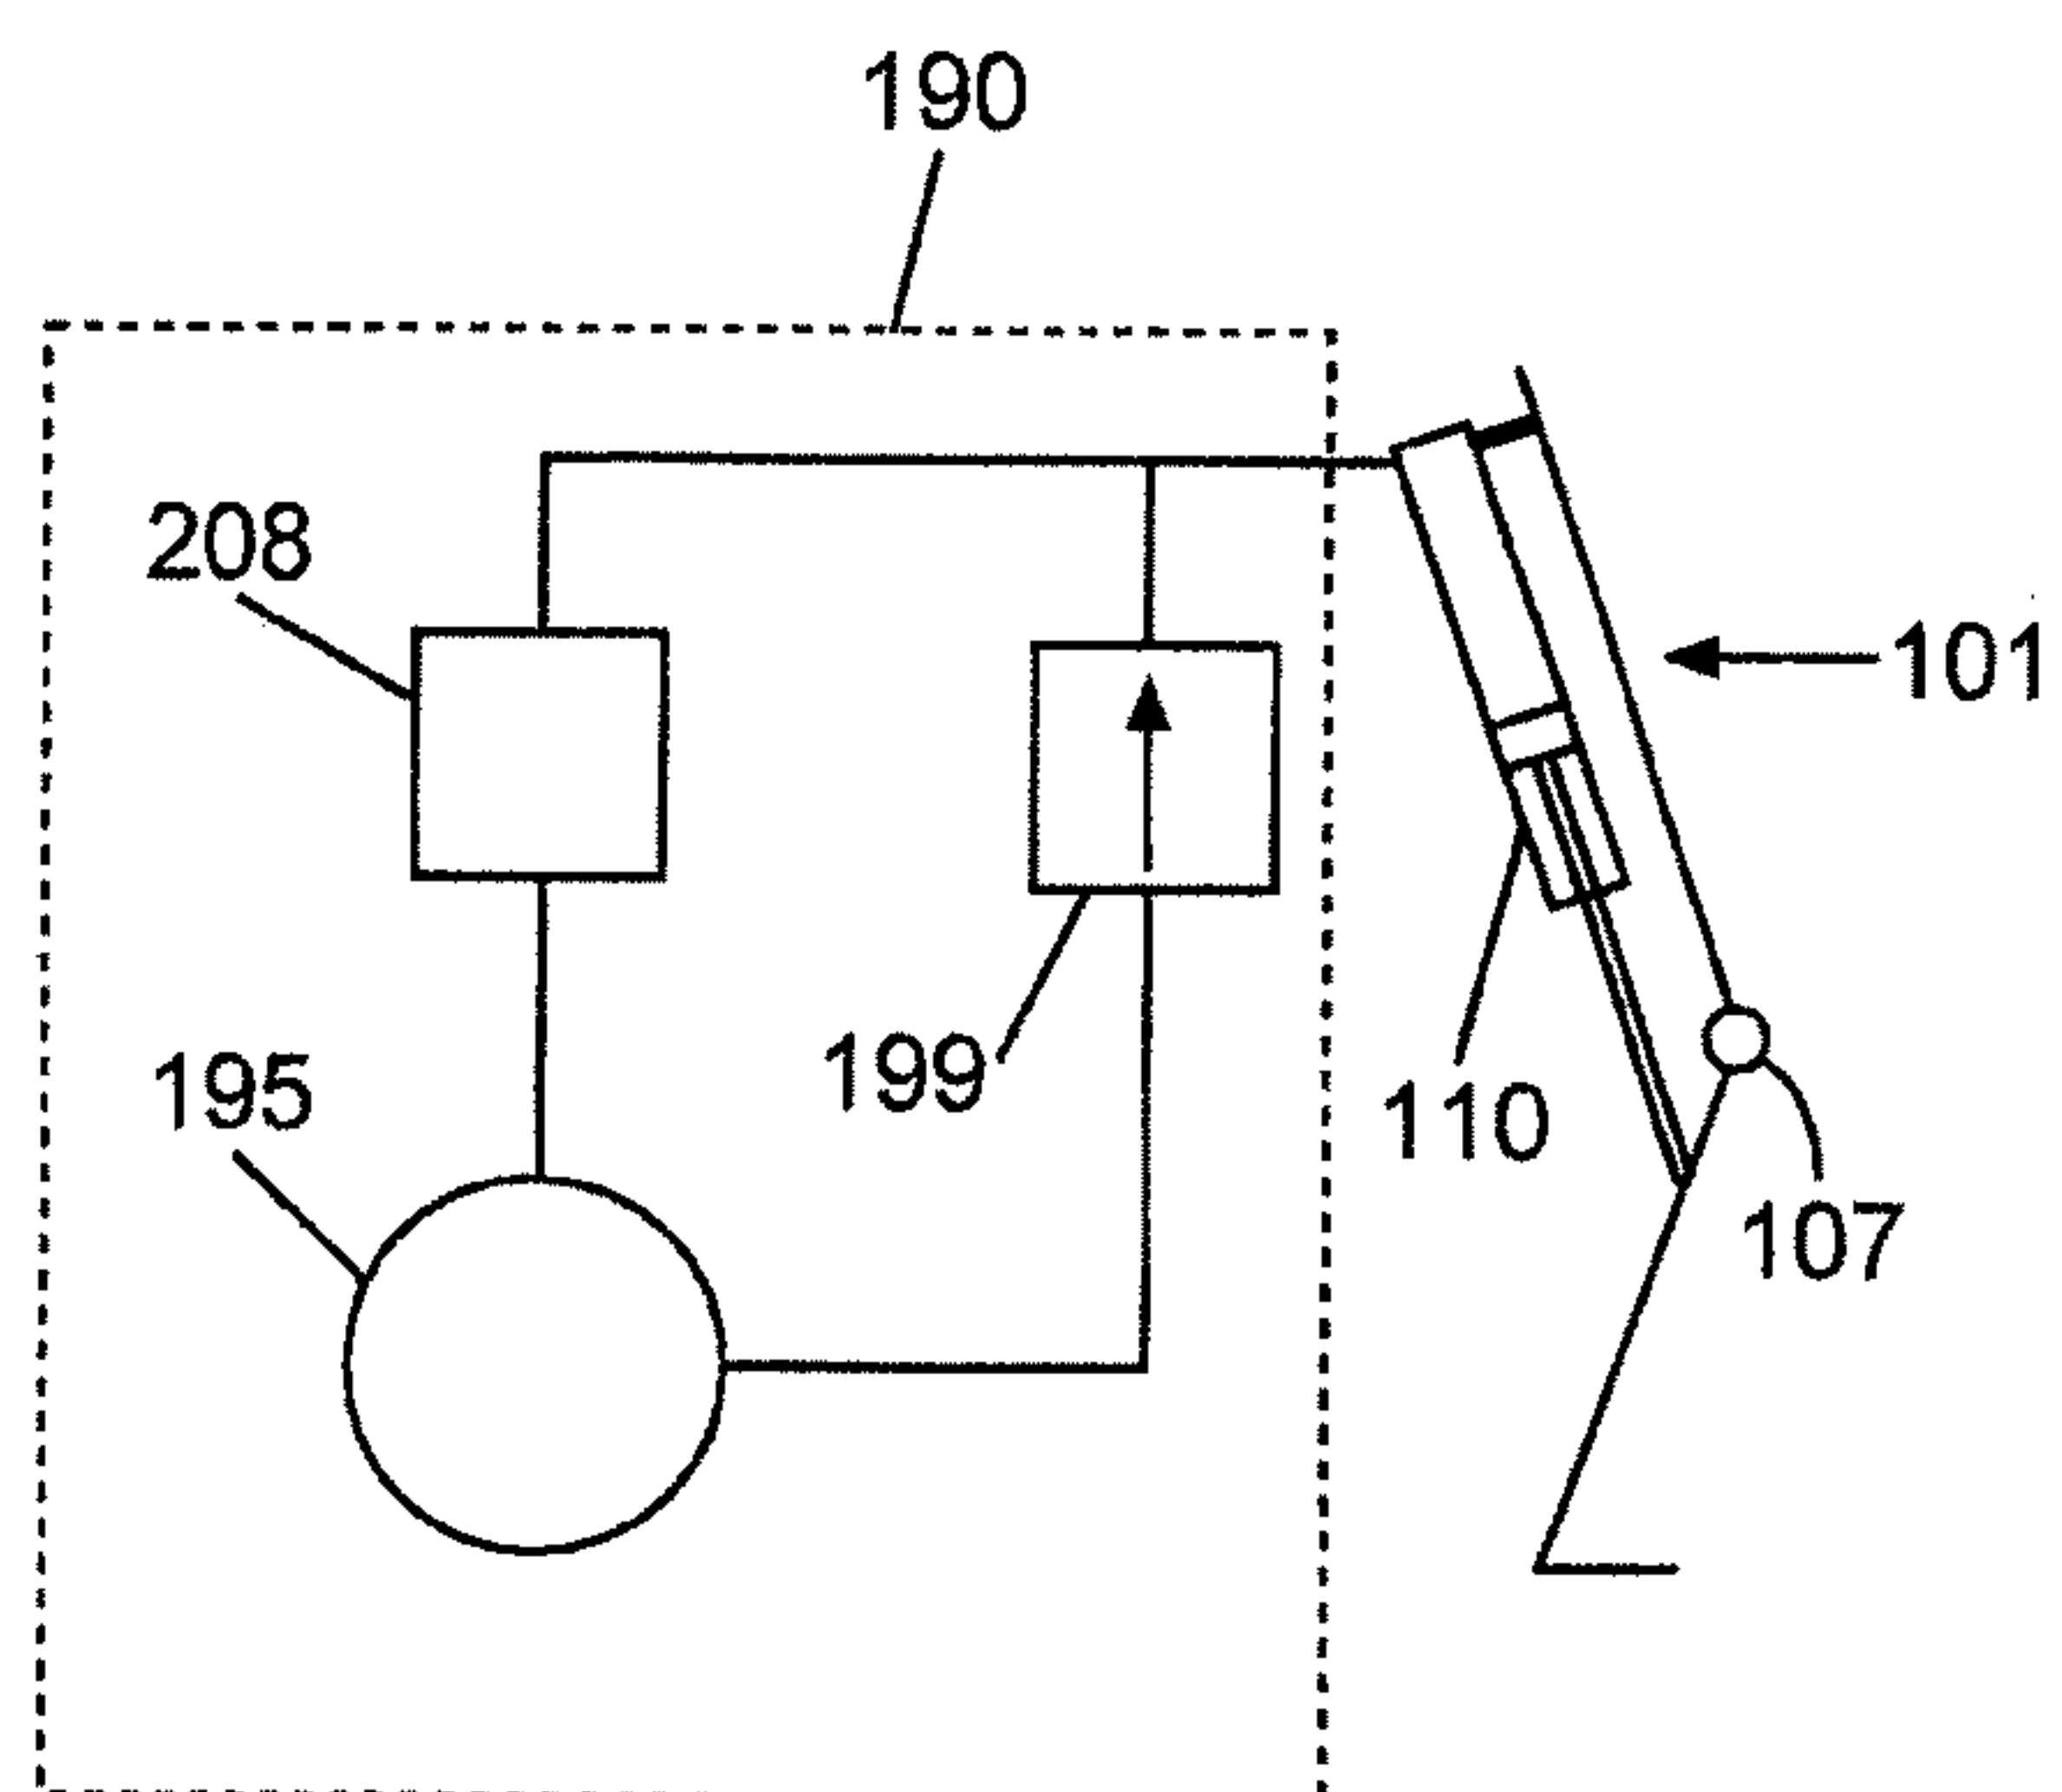


Figure 38

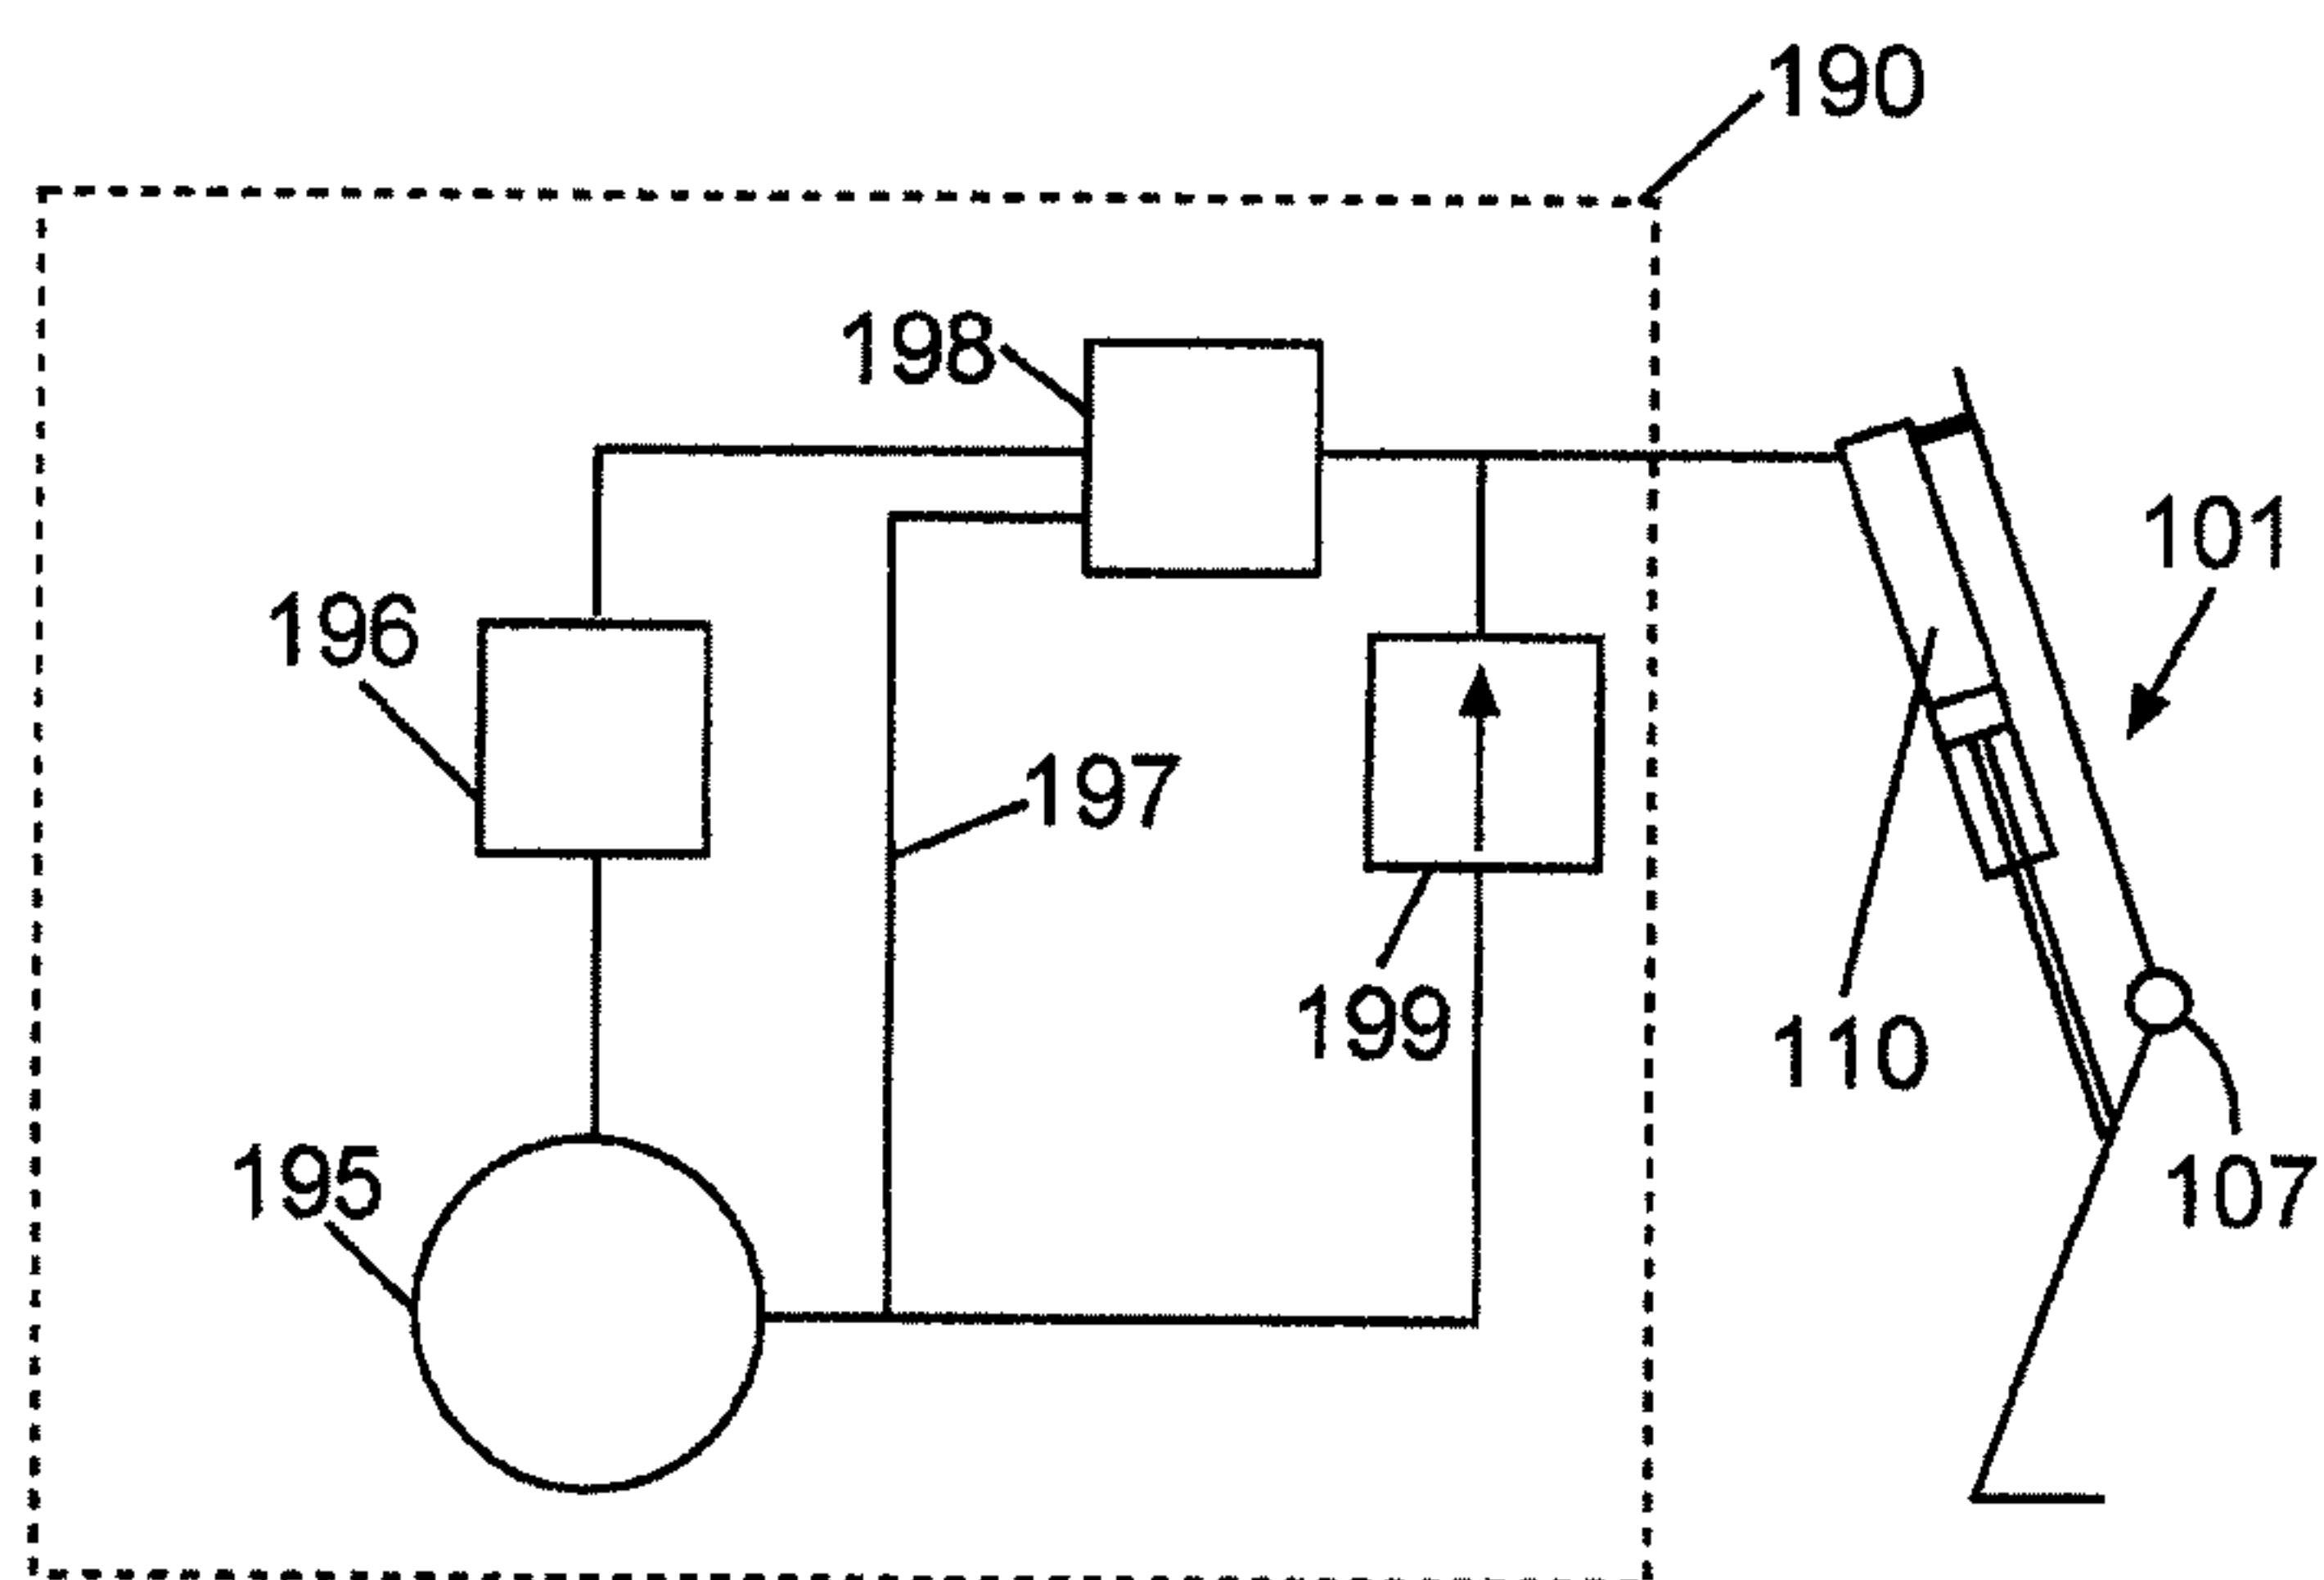


Figure 39

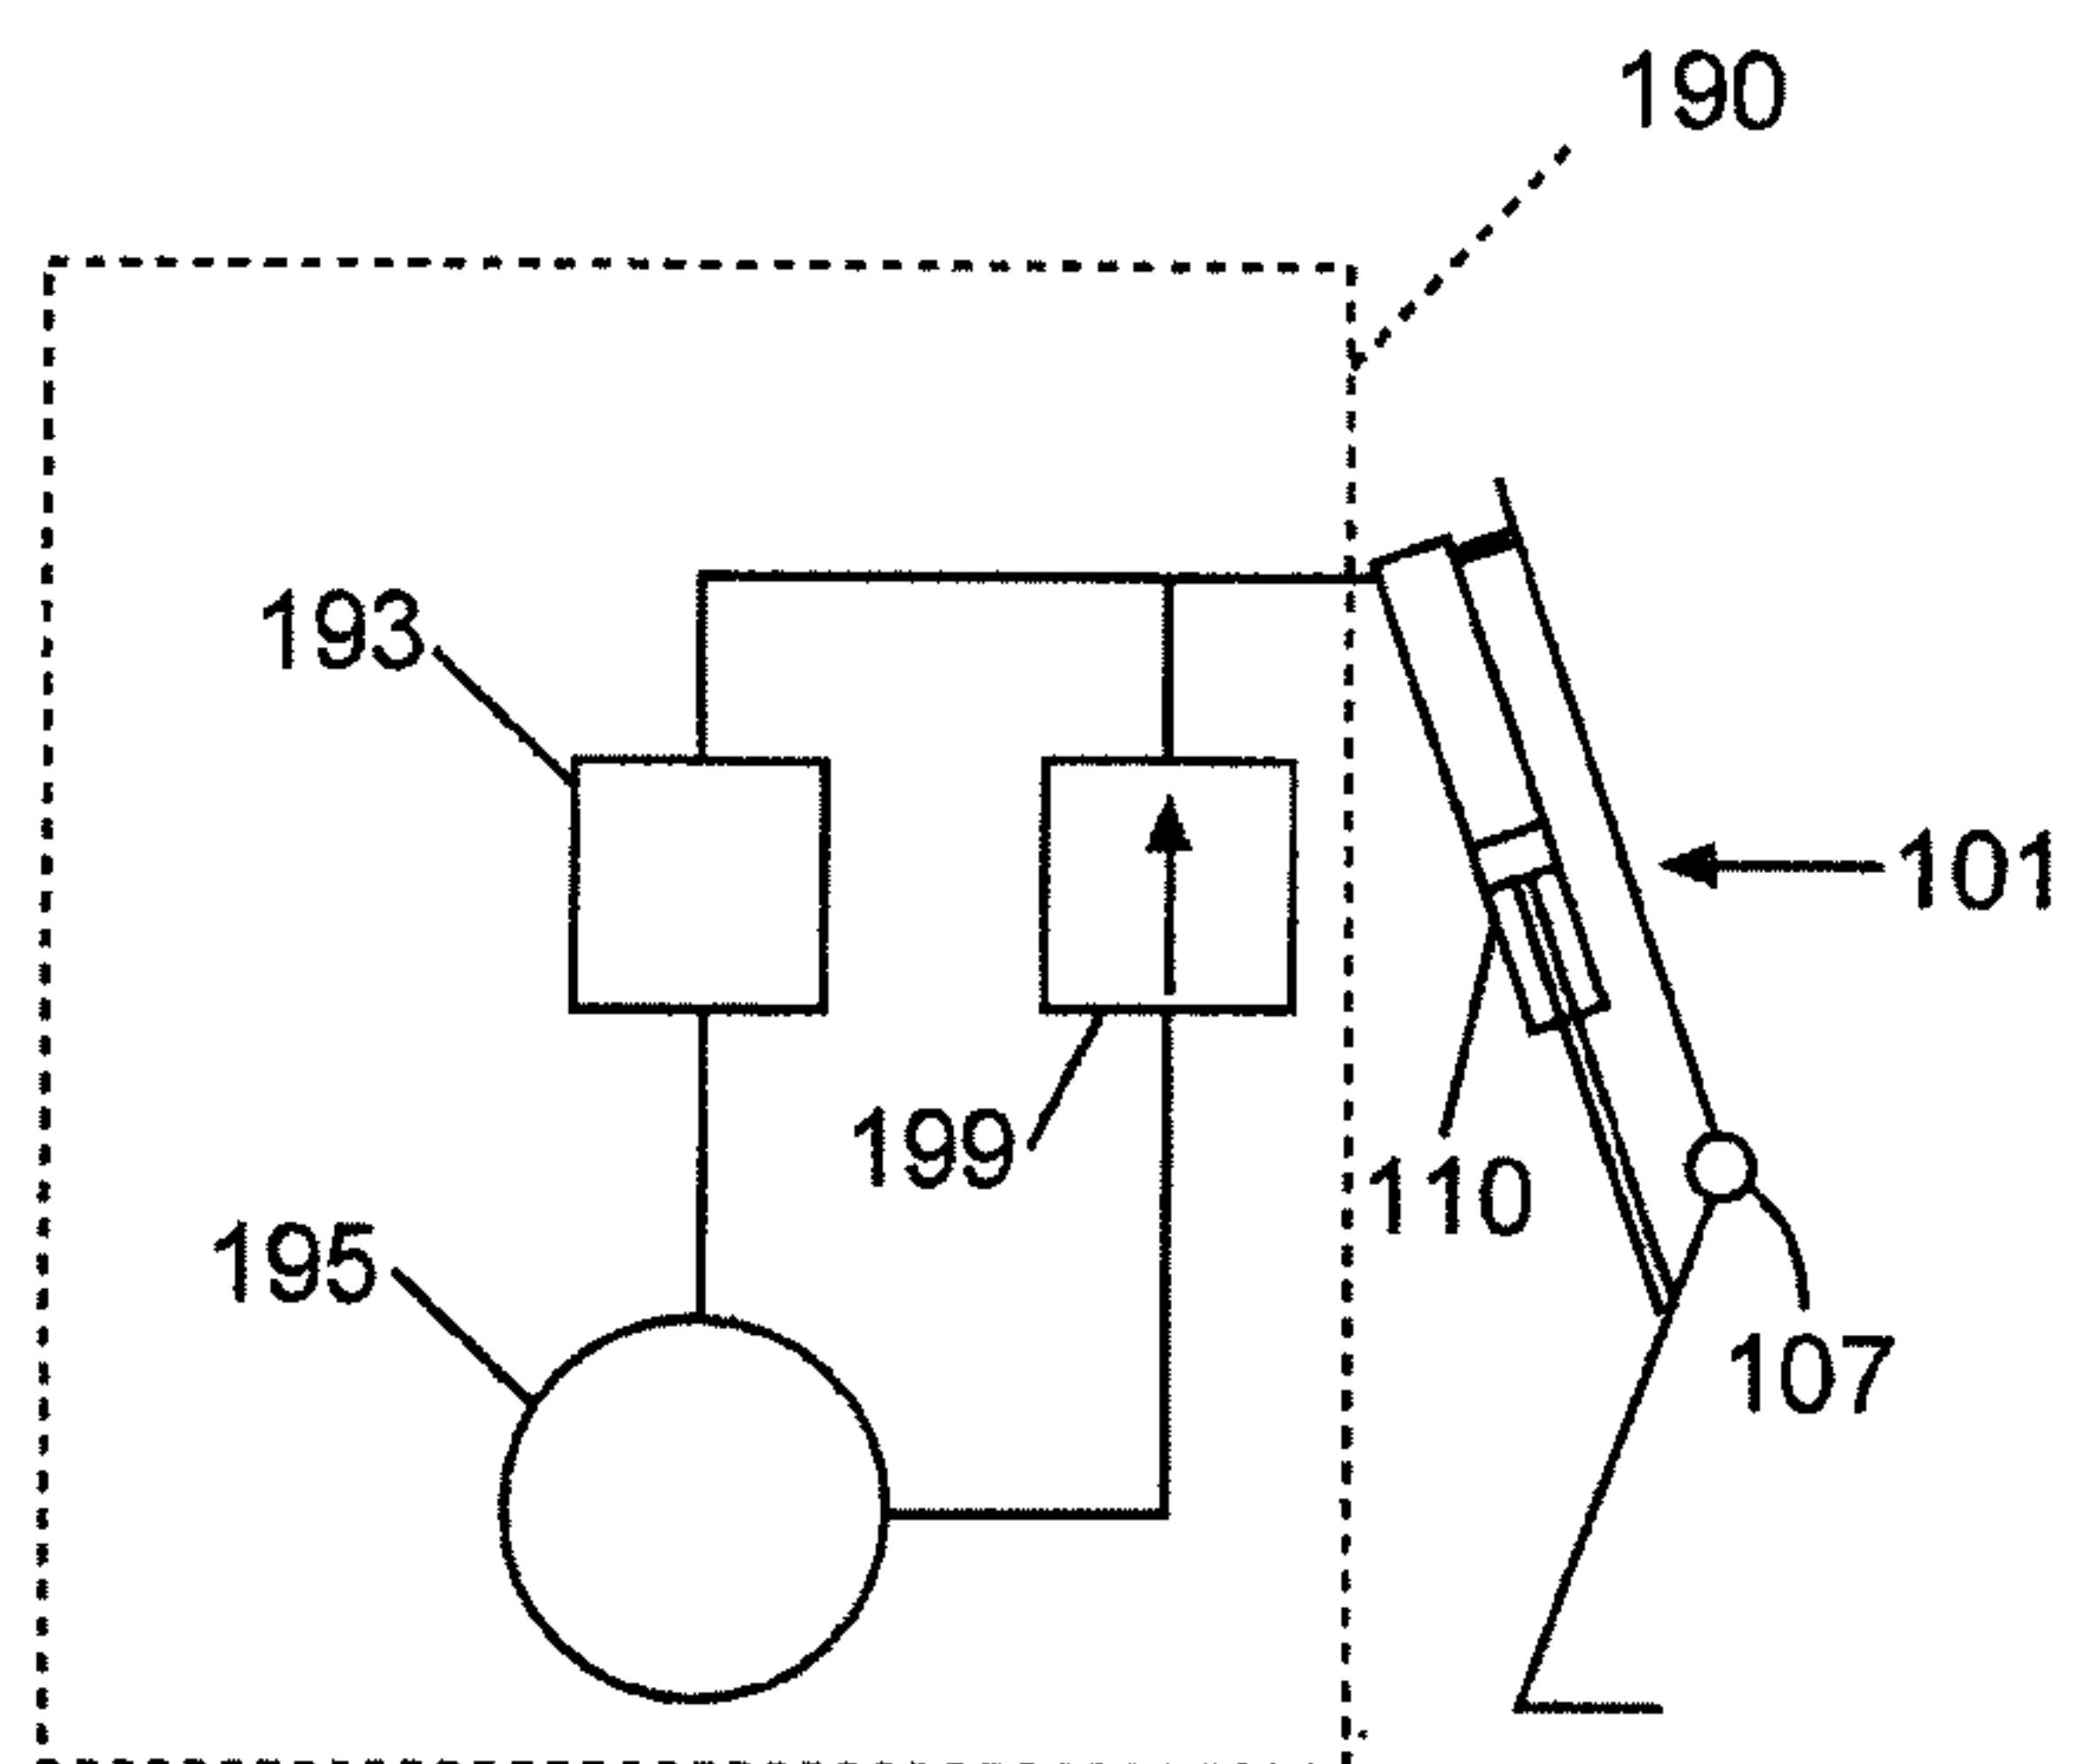


Figure 40

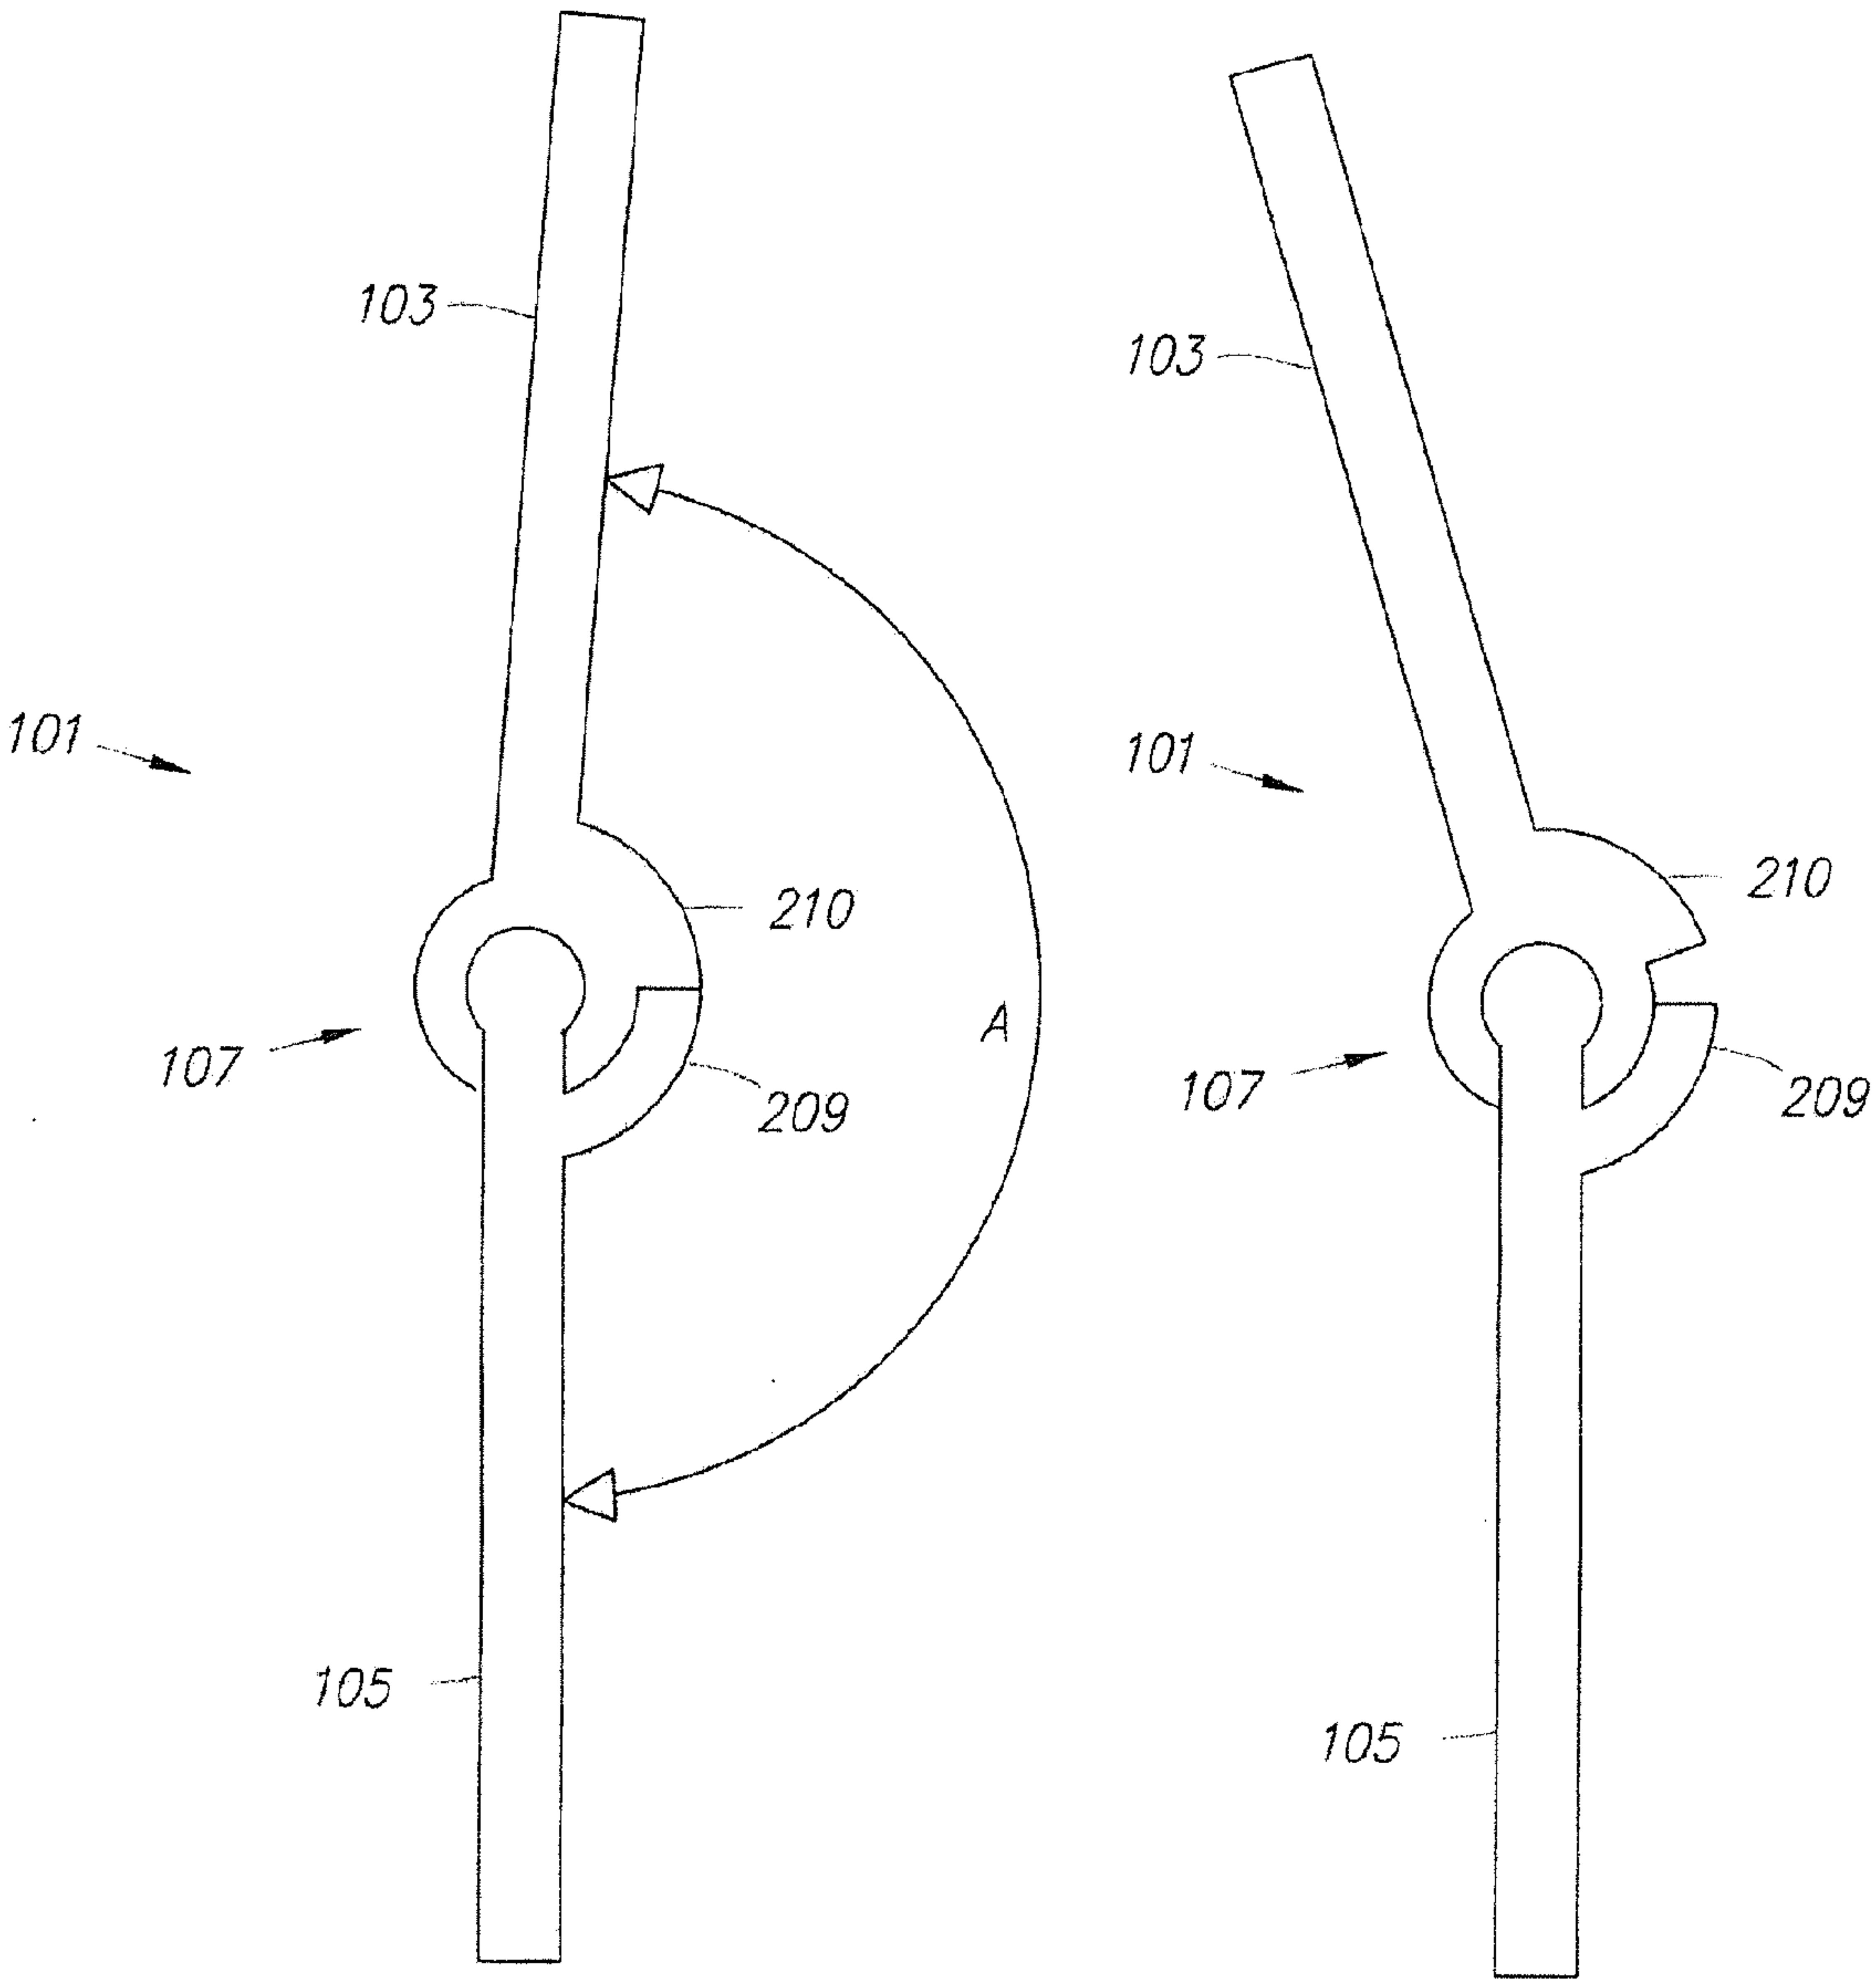


Fig. 41

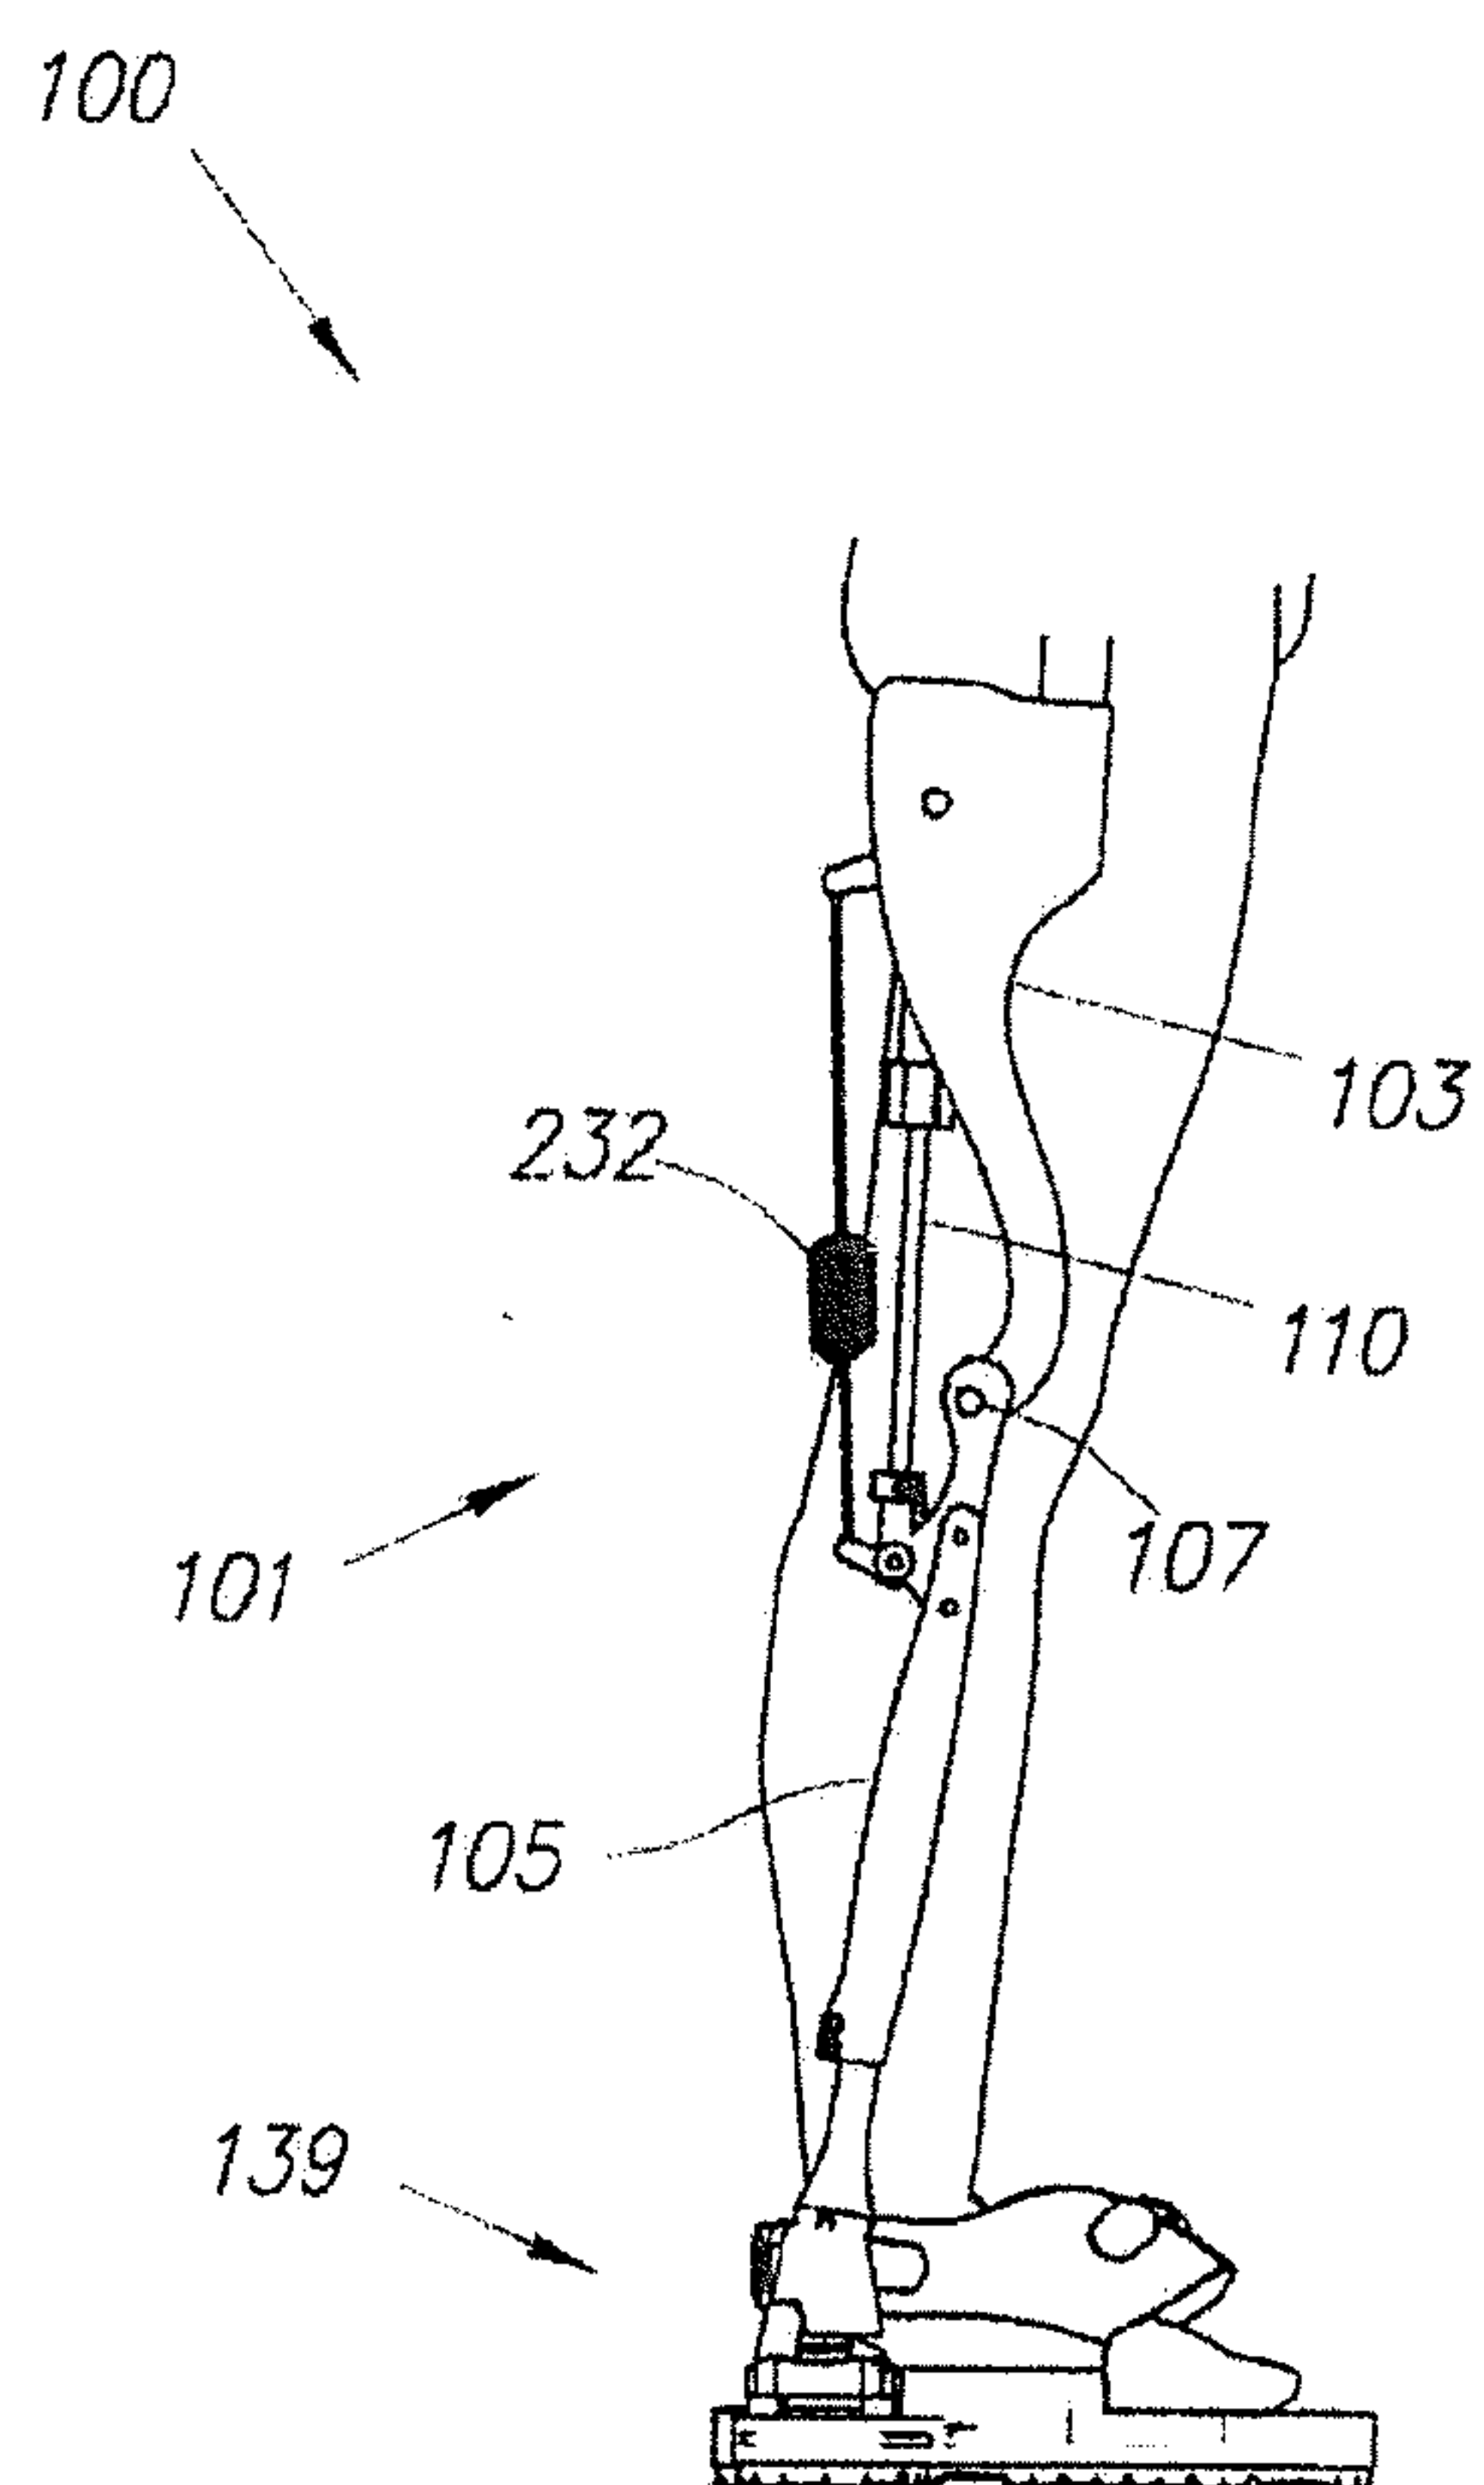


Fig. 42

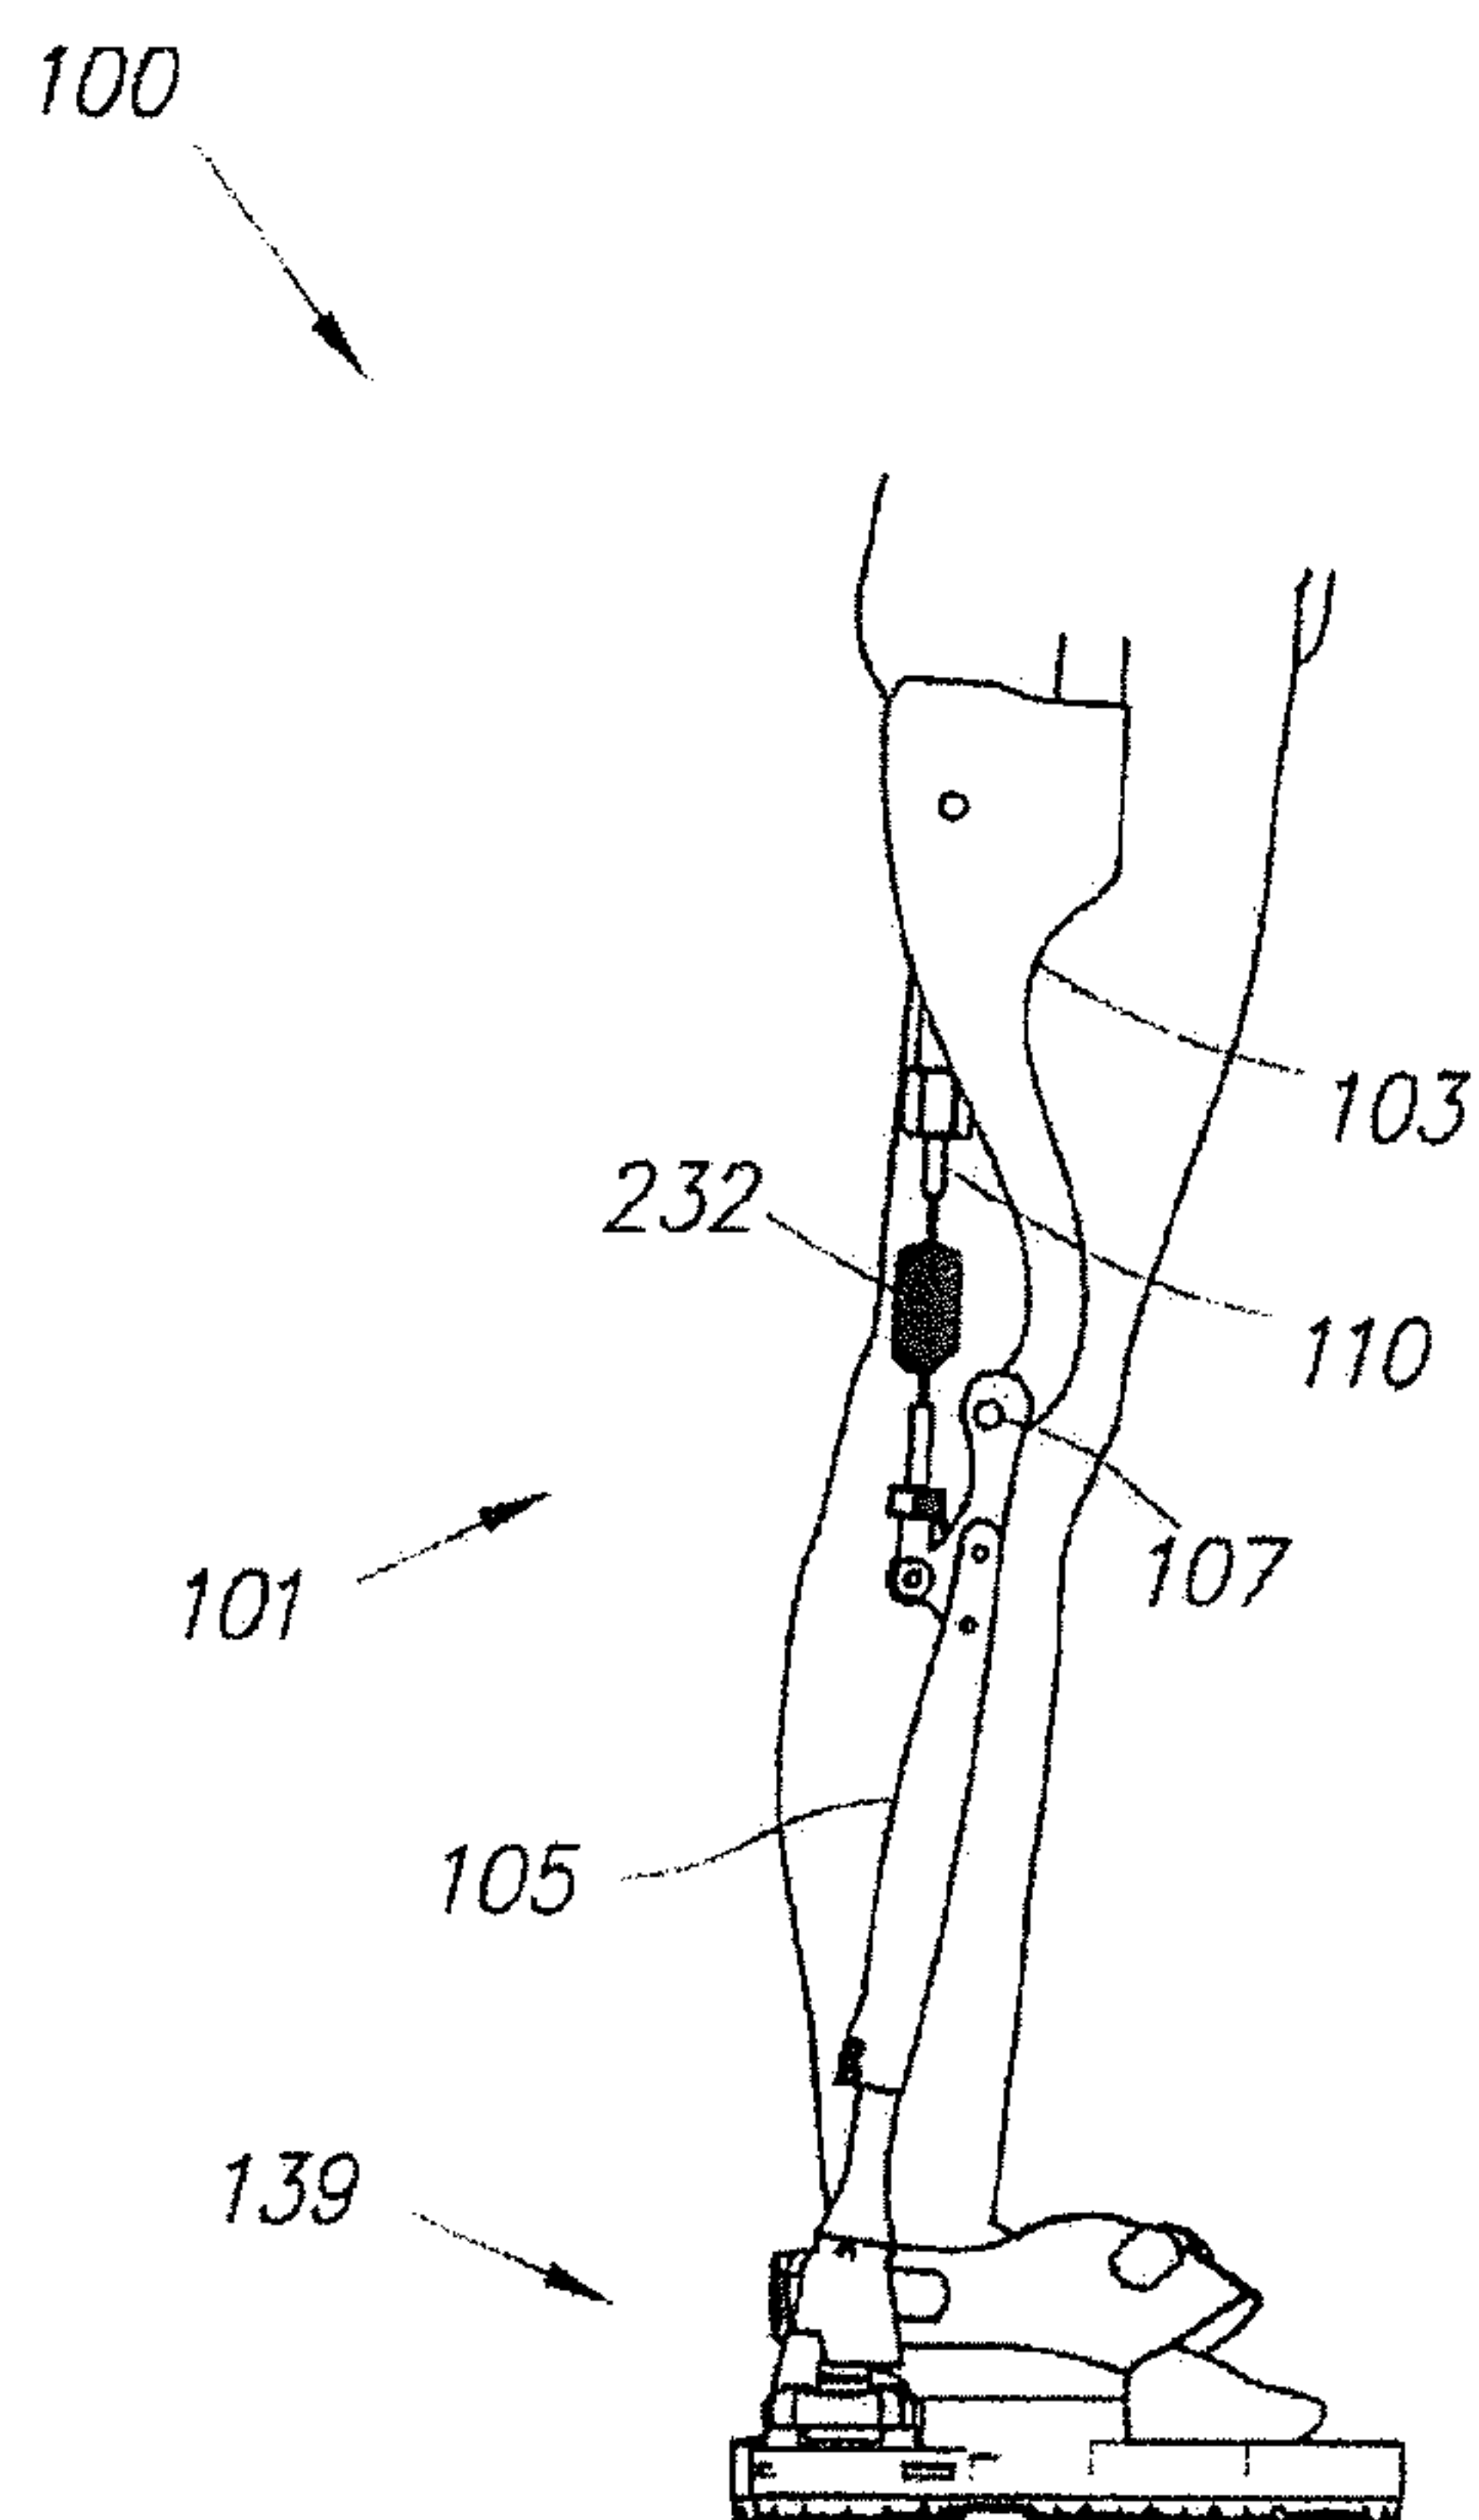


Fig. 43


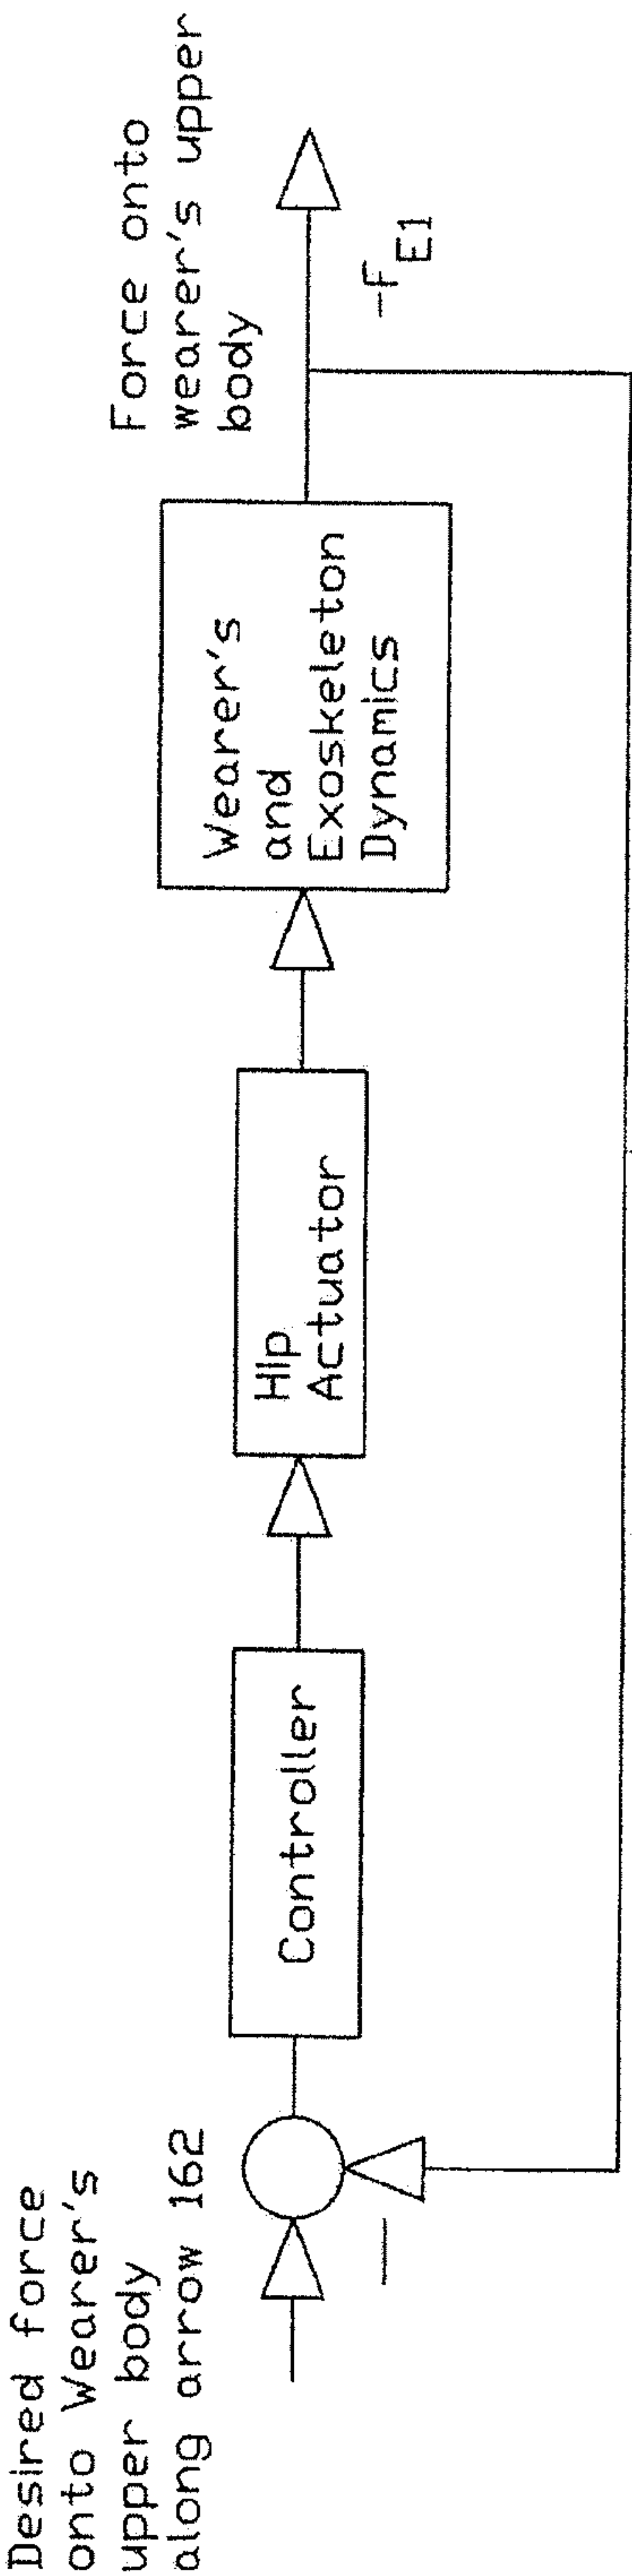


Fig. 44

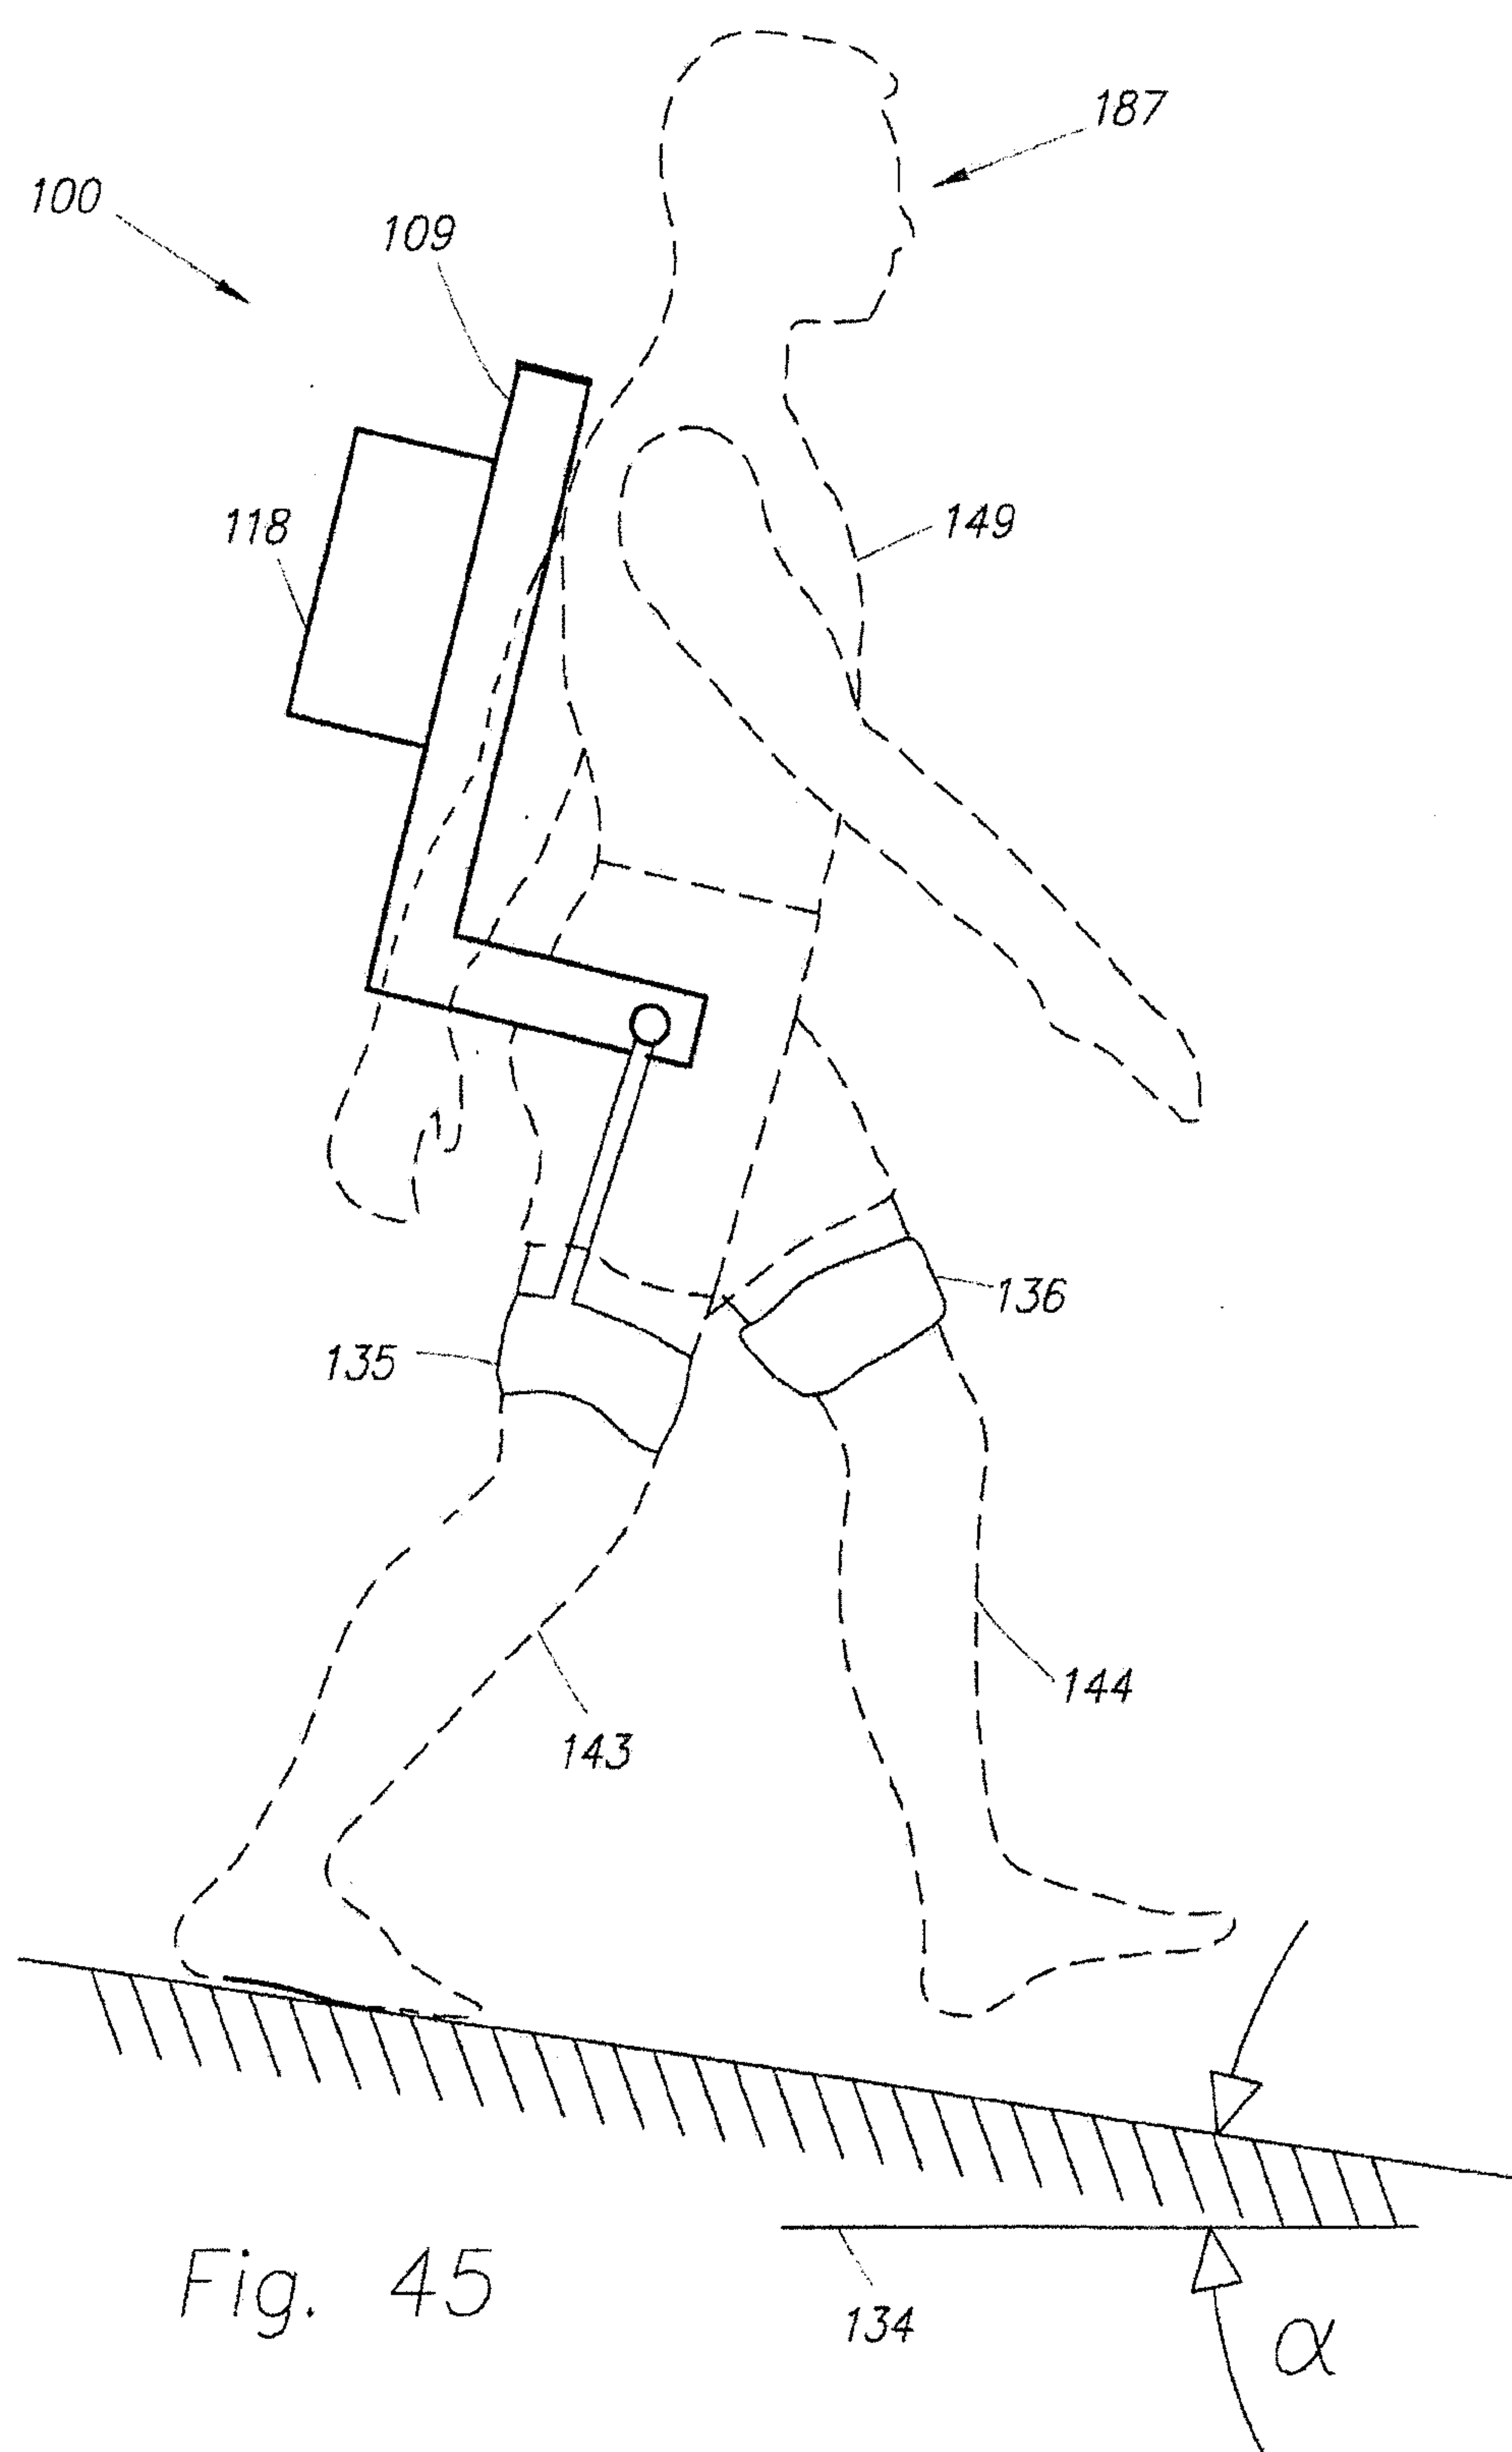

**DEVICE AND METHOD FOR DECREASING
ENERGY CONSUMPTION OF A PERSON BY
USE OF A LOWER EXTREMITY
EXOSKELETON**

CROSS-REFERENCE TO RELATED
APPLICATIONS

[0001] This application represents a continuation of pending U.S. patent application Ser. No. 12/468,595, filed May 19, 2009 which claims the benefit of U.S. Provisional Application No. 61/071,823 entitled DEVICE AND METHOD FOR DECREASING ENERGY CONSUMPTION OF A PERSON BY USE OF A LOWER EXTREMITY EXOSKELETON, filed May 20, 2008.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] The present invention relates generally to the field of lower extremity exoskeletons and, more particularly, to the field of lower extremity exoskeletons that decrease their wearer's energy consumption.

[0004] 2. Discussion of the Prior Art

[0005] In a wide variety of situations, people of ordinary ability often consume a great deal of energy when walking or carrying a load. One attempt to improve load carrying ability is set forth in the paper entitled "A QUASI-PASSIVE LEG EXOSKELETON FOR LOAD-CARRYING AUGMENTATION", C. J. Walsh, K. Endo, and H. Herr, International Journal of Humanoid Robotics, 2007. However, the quasi-passive exoskeleton taught by Walsh et al. increases its wearer's oxygen consumption. More specifically, the exoskeleton described has no actuation and power unit and therefore will not be able to transfer power from the exoskeleton to the person. This means that this type of system, regardless of the location and strength of its springs, will not decrease its wearer's energy expenditure. Since oxygen consumption is proportional to energy expended, a wearer's oxygen consumption will not be decreased.

[0006] An article published by Popular Science Magazine (May 2008) describes a powered exoskeleton system designed and built by Sarcos, that is controlled by a method called "get out of the way". This method measures the forces and torques a wearer exerts onto the exoskeleton and drives the exoskeleton based on these measurements. This "get out of the way" control method has been extensively used in control of intelligent assist devices. See U.S. Pat. Nos. 6,299,139, 6,386,513, and 6,886,812. However, the "get out of the way" control method will not reduce a wearer's energy expenditure because the force from the exoskeleton onto the wearer is in the opposite direction to the wearer's motion and in fact increases the wearer's energy expenditure.

[0007] Based on the above, opportunities exist to provide a general purpose exoskeleton device that will decrease the wearer's energy consumption while the device is worn. Providing an exoskeleton that decreases the energy consumption of its wearer would allow a wearer to walk and carry heavy objects, while reducing the wearer's energy expenditure. In particular, this invention covers various embodiments of exoskeleton devices that decrease their wearers' energy expenditure during a stance phase.

SUMMARY OF THE INVENTION

[0008] The opportunities described above are addressed in several embodiments of a lower extremity exoskeleton, wearable by a person. The lower extremity exoskeleton described here is configurable to be coupled to a person and, among other components, comprises: two leg supports configurable to be coupled to the person's lower limbs; two knee joints, each of which is configured to allow flexion and extension between a respective shank link and respective thigh link; an exoskeleton trunk, which is configurable to be coupled to the person's upper body and is rotatably connectable to the thigh links of the leg supports, allowing for the flexion and extension between the leg supports and the exoskeleton trunk; two hip actuators, which are configured to create torques between the exoskeleton trunk and leg supports; and at least one power unit, which is capable of providing power to the hip actuators, among other components. In operation, when the lower extremity exoskeleton is worn by the person, one leg support is in the stance phase and the other leg support is in the swing phase, the power unit is configured to cause the hip actuator of the leg support in the stance phase to create a torque profile such that the energy supplied by the power unit to the hip actuator of the leg support in stance phase is greater than the energy required to move the exoskeleton trunk and the leg support in stance phase through the same trajectory when not worn by the person.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] These and other features, aspects, and advantages of the present invention will become better understood when the following detailed description is read with reference to the accompanying drawings, in which like characters represent like parts throughout the drawings, wherein:

[0010] FIG. 1 is a front perspective drawing of an exoskeleton of the present invention;

[0011] FIG. 2 is a rear perspective drawing of the exoskeleton of FIG. 1.

[0012] FIG. 3 depicts an alternative exoskeleton of the present invention in a stance phase;

[0013] FIG. 4 depicts the exoskeleton of FIG. 3 moving in a forward velocity direction during the stance phase;

[0014] FIG. 5 depicts forces and dimensions associated with the exoskeleton of FIG. 3 in the stance phase;

[0015] FIG. 6 is a schematic drawing of a power unit of the present invention;

[0016] FIG. 7 is a schematic drawing of an alternative power unit of the present invention including a flow restrictive valve;

[0017] FIG. 8 is a schematic drawing of an alternative power unit of the present invention including a three-way valve;

[0018] FIG. 9 is a perspective drawing of an alternative exoskeleton of the present invention including stance sensors in communication with a signal processor;

[0019] FIG. 10 is a perspective drawing of an alternative exoskeleton of the present invention including a hip resilient element;

[0020] FIG. 11 is a perspective drawing of an alternative exoskeleton of the present invention including a connecting bracket for carrying a rear load;

[0021] FIG. 12 is a perspective drawing of an alternative exoskeleton of the present invention including extension frames for carrying a front load;

[0022] FIG. 13 is a perspective drawing of an alternative exoskeleton of the present invention including a hip abduction stop;

[0023] FIG. 14 is a perspective drawing of an alternative exoskeleton of the present invention including a hip resilient element in the form of a leaf spring;

[0024] FIG. 15 is a perspective drawing of an alternative exoskeleton of the present invention including two hip resilient elements;

[0025] FIG. 16 is a perspective drawing of an alternative exoskeleton of the present invention including two hip joints;

[0026] FIG. 17 is a perspective drawing of an alternative exoskeleton of the present invention including a back pack frame;

[0027] FIG. 18 is a perspective drawing of an alternative exoskeleton of the present invention including two hip resilient elements and exoskeleton feet;

[0028] FIG. 19 is a partial view of the exoskeleton of FIG. 18, showing thigh joint details;

[0029] FIG. 20 is a partial view of the exoskeleton of FIG. 18, showing details of a compression-elongation mechanism;

[0030] FIG. 21 is a perspective drawing of an alternative exoskeleton of the present invention including shoes;

[0031] FIG. 22 is a perspective drawing of an alternative exoskeleton of the present invention including insoles;

[0032] FIG. 23 is partial view of an exoskeleton foot of FIG. 18 including a ball and socket joint;

[0033] FIG. 24 is a perspective drawing of an alternative exoskeleton foot of the present invention including resilient elements;

[0034] FIG. 25 is a perspective drawing of an alternative exoskeleton foot of the present invention including an abduction-adduction resilient element;

[0035] FIG. 26 is a perspective drawing of an alternative exoskeleton foot of the present invention including a shank rotating joint;

[0036] FIG. 27 depicts forces and dimensions associated with an alternative exoskeleton of the present invention in a stance phase;

[0037] FIG. 28 is a partial cross-sectional side view of an alternative exoskeleton foot of the present invention including an integrated stance sensor;

[0038] FIG. 29 is a top perspective view of an alternative exoskeleton foot of the present invention including a force sensor;

[0039] FIG. 30 is a partial cross-sectional side view of an alternative shoe of the present invention including an integrated stance sensor;

[0040] FIG. 31 is a partial cross-sectional side view of an alternative shoe of the present invention including a sole-mounted stance sensor;

[0041] FIG. 32 is a partial cross-sectional side view of an alternative shoe of the present invention including a force sensor incorporated into the shoe sole;

[0042] FIG. 33 is a side view of an alternative exoskeleton of the present invention carried in a vertical stowed position;

[0043] FIG. 34 is a partial perspective view of the exoskeleton of FIG. 33;

[0044] FIG. 35 is a perspective drawing of an alternative exoskeleton foot of the present invention including hydraulic rotary dampers;

[0045] FIG. 36 is a schematic drawing of a knee hydraulic circuit of the present invention;

[0046] FIG. 37 is a schematic drawing of an alternative knee hydraulic circuit of the present invention including a three-way valve;

[0047] FIG. 38 is a schematic drawing of an alternative knee hydraulic circuit of the present invention including a check valve;

[0048] FIG. 39 is a schematic drawing of an alternative knee hydraulic circuit of the present invention including a three-way valve and a check valve;

[0049] FIG. 40 is a schematic drawing of an alternative knee hydraulic circuit of the present invention including a two-way valve and a check valve;

[0050] FIG. 41 depicts the function of a locking knee joint in accordance with the present invention;

[0051] FIG. 42 is a side view of an alternative right leg support of the present invention including knee resilient elements in parallel with torque generators;

[0052] FIG. 43 is a side view of an alternative right leg support of the present invention including knee resilient elements in series with torque generators;

[0053] FIG. 44 is a diagram depicting the use of a closed loop controller to control force applied in accordance with the present invention; and

[0054] FIG. 45 is a side view of an alternative exoskeleton of the present invention including legs which do not touch the ground.

DETAILED DESCRIPTION OF THE INVENTION

[0055] In accordance with an embodiment of the present invention, FIG. 1 is a perspective drawing illustrating a lower extremity exoskeleton 100 wearable by a person 187 that is able to decrease the wearer's energy consumption during walking. Lower extremity exoskeleton 100, in addition to other components, includes two leg supports, 101 and 102, which are configured to be coupled to person's lower limbs 143 and 144, and is configured to rest on a support surface (e.g., the ground) during their stance phase. The term stance phase should be understood to mean the position a leg support 101 or 102 is in when a force is being applied to a user's foot and leg associated with the leg support 101 or 102. The leg supports, in addition to other components, includes thigh links 103 and 104 and shank links 105 and 106. Two knee joints, 107 and 108, are configured to allow flexion and extension between the shank link and the thigh link of the leg supports (shown by knee flexion arrow 213 and knee extension arrow 214, respectively) during the corresponding leg support swing phase. The term swing phase should be understood to mean the position a leg support 101 or 102 is in when a force is not be applied to a user's foot and leg associated with the leg support 101 or 102. However, two knee joints, 107 and 108, in some embodiments are configured to resist flexion between the shank link and the thigh link of the leg supports during the corresponding leg support stance phase. Lower extremity exoskeleton 100, among other components, further comprises an exoskeleton trunk 109. Exoskeleton trunk 109, among other components, comprises an upper body interface device 150. Exoskeleton trunk 109 is configurable to be coupled to the person's upper body 149 through upper body interface device 150. Person's upper body 149 means any location generally above the thighs, including the buttock. Examples of upper body interface device 150 comprise an element or combination of elements including, without limitation, vests, belts, straps, shoulder straps, chest straps, body cast, harness, and waist belts. Exoskeleton trunk

109 is rotatably connectable to leg supports **101** and **102** at hip flexion-extension joints **125** and **126**, allowing for the hip flexion and extension rotations (shown by hip extension arrow **215** and hip flexion arrow **216**, respectively) of leg supports **101** and **102** about hip flexion-extension axes **151** and **152**, respectively. Leg supports **101** and **102** are configurable to be coupled to person's lower limbs **143** and **144** through lower limb interface straps **135** and **136**. Person's lower limbs **143** and **144** should be understood to mean any location generally below the thighs. In some embodiments, as shown in FIG. 1, lower limb interface straps **135** and **136** are coupled to thigh links **103** and **104**. In some embodiments, as shown in FIG. 2, lower limb interface straps **135** and **136** are coupled to shank links **105** and **106**. In some embodiments, lower limb interface straps are coupled to both shank links and thigh links. Each lower limb interface strap **135** and **136** comprises an element or combination of elements including, without limitation, straps, bars, c-shaped brackets, body cast, and elastomers. In operation, person **187** is coupled to (or wears) lower extremity exoskeleton **100** through upper body interface device **150** (a simple belt in the case of FIG. 1) and by coupling to two leg supports **101** and **102** through lower limb interface straps **135** and **136**.

[0056] Lower extremity exoskeleton **100**, among other things, further comprises two hip actuators **145** and **146** which are configured to create torques between exoskeleton trunk **109** and leg supports **101** and **102**. Right hip actuator **145** is shown in FIG. 1 and left hip actuator **146** is shown in FIG. 2. Lower extremity exoskeleton **100**, among other components, further comprises at least one power unit **201** capable of providing power and is coupled to hip actuators **145** and **146**. In some embodiments, only one power unit **201** provides power to hip actuators **145** and **146**. In some embodiments, each hip actuator receives power from separate power units. Hip actuators **145** and **146** comprise any device or combination of devices capable of providing torque. Examples of hip actuators **145** and **146** include, without limitation, electric motors, including, without limitation, AC (alternating current) motors, brush-type DC (direct current) motors, brushless DC motors, electronically commutated motors (ECMs), stepping motors, hydraulic actuators, and pneumatic actuators and combinations thereof. In some embodiments, hip actuators **145** and **146** are powered by compressed gas. In some embodiments, exoskeleton trunk **109** is configured to hold a rear load behind person **187**.

[0057] FIG. 3 shows a configuration of lower extremity exoskeleton **100** where right leg support **101** and person's right lower limb **143** are in the stance phase, and left leg support **102** and person's left lower limb **144** are in the swing phase (left leg support **102** is not shown in FIG. 3). Please note that exoskeleton trunk **109**, in this embodiment, has been designed to extend along a person's back to hold a rear load **118**. Further note that the following analysis clearly applies to the reverse configuration where right leg support **101** is in swing phase and left leg support **102** is in stance phase. FIG. 4 shows three configurations of lower extremity exoskeleton **100** during a stance phase of right leg support **101** when a wearer is moving in a forward velocity direction **162**. These configurations are shown by letters A (beginning of the single stance phase), B (somewhere in the middle of the single stance phase), and C (end of the single stance phase) of right leg support **101**. Based on our observations, we have concluded that a person's upper body **149** and exoskeleton trunk **109** move with little rotation, which results in a relatively

constant angle of the persons' upper body **149** and exoskeleton trunk **109** with respect to ground **130**.

[0058] In operation, when right leg support **101** is in the stance phase and left leg support **102** is in the swing phase, power unit **201** is configured to cause the corresponding right hip actuator **145** of right leg support **101** to create a torque profile. Because of this torque profile, lower extremity exoskeleton **100** and person **187** travel from configuration A to configuration C (as shown in FIG. 4), where right leg support **101** and person's right lower limb **143** are in the stance phase. The person's forward velocity direction **162** is generally parallel with ground **130**. During the stance phase of right leg support **101**, mechanical work $W_{ACTUATOR}$ is produced by right hip actuator **145** during the time that lower extremity exoskeleton **100** and person **187** travel from configuration A to configuration C. The total mechanical energy (kinetic energy plus potential energy) of right leg support **101** and exoskeleton trunk **109**, including any load on exoskeleton trunk **109** (i.e., lower extremity exoskeleton **100** without the swinging left leg support **102**), at configuration A is denoted by E_A . The total mechanical energy (kinetic energy plus potential energy) of right leg support **101** and exoskeleton trunk **109**, including any load on exoskeleton trunk **109**, (i.e., lower extremity exoskeleton **100** without the swinging left leg support **102**) at configuration C is denoted by E_C . The energy wasted to friction and other losses during the stance phase of right leg support **101** are denoted by E_{LOSS} . If $W_{ACTUATOR} > (E_C - E_A + E_{LOSS})$, then energy is transferred to person **187** from lower extremity exoskeleton **100** and is equal to $[W_{ACTUATOR} - (E_C - E_A + E_{LOSS})]$. If $W_{ACTUATOR} < (E_C - E_A + E_{LOSS})$, then energy is transferred from person **187** to lower extremity exoskeleton **100** and is equal to $[(E_C - E_A + E_{LOSS}) - W_{ACTUATOR}]$.

[0059] In summary:

If $W_{ACTUATOR} > (E_C - E_A + E_{LOSS})$, energy transferred to person **187** = $W_{ACTUATOR} - (E_C - E_A + E_{LOSS})$

[0060] If $W_{ACTUATOR} < (E_C - E_A + E_{LOSS})$, energy transferred from person **187** = $(E_C - E_A + E_{LOSS}) - W_{ACTUATOR}$

[0061] The required energy to move exoskeleton trunk **109** and right leg support **101** through the same trajectory from A to C when exoskeleton **100** is not worn by person **187** is $(E_C - E_A + E_{LOSS})$. This means that, to transfer energy to person **187** during the stance phase of right leg support **101**, the energy supplied by power unit **201** to right hip actuator **145** of right leg support **101** must be larger than the energy required to move exoskeleton trunk **109** and right leg support **101** through the same trajectory from A to C when person **187** is not present. An incremental increase in mechanical energy transferred to person **187** during the stance phase will result in an incremental decrease in wearer's energy required for locomotion during the stance phase. Since the wearer's oxygen consumption is proportional with the energy expenditure, a decrease in the wearer's energy required for locomotion leads to less oxygen consumption by the wearer. One way to ensure mechanical energy is transferred to person **187** during the stance phase is to ensure that the torque profile of right hip actuator **145** of right leg support **101** is generally larger than the torque required to move exoskeleton trunk **109** and right leg support **101** through the same trajectory from A to C when person **187** is not present. This is described below with the help of FIG. 4 and FIG. 5.

[0062] FIG. 5 shows a configuration of lower extremity exoskeleton 100 when right leg support 101 is in the stance phase (the same configuration as FIG. 3 without the person drawn). Ground 130 has a slope of α with the horizontal ground 134. Person's upper body 149 is coupled to exoskeleton trunk 109 through upper body interface device 150. Based on our observations, we have noticed that person's upper body 149 and exoskeleton trunk 109 move with little rotation (compared to variation of hip angle λ). This means that the angle of the person's upper body 149 and exoskeleton trunk 109 with respect to ground 130 remains relatively constant during the stance phase of right leg support 101. β_2 represents the angle between ground 130 and a line perpendicular to exoskeleton trunk 109, as shown in FIG. 5. Based on the observations described above, β_2 is relatively constant in comparison to angle λ . During the stance phase, right thigh link 103 and right shank link 105 move very little or not at all relative to each other. This means right leg support 101 during the stance phase can be approximated like a rigid link swinging from position A to position C, as shown in FIG. 4.

[0063] The Kinetic energy and the Potential energy of the system shown in FIG. 4 are expressed by equations (1) and (2).

$$\text{Kinetic Energy} = \frac{(M_{TRUNK}L^2 + I)\dot{\beta}_1^2}{2} \quad (1)$$

$$\text{Potential Energy} = (LM_{TRUNK} + RM_L)g\cos(\beta_1 + \alpha) + K \quad (2)$$

where:

[0064] M_{TRUNK} : mass of exoskeleton trunk 109 and any attached load (e.g., rear load 118)

[0065] M_L : mass of right leg support 101

[0066] I : moment of inertia of right leg support 101 about point F

[0067] L : length of right leg support 101 during stance as shown in FIG. 5

[0068] R : distance between the center of mass of right leg support 101 and point F (not shown in any figure)

[0069] β_1 : the angle between ground 130 and a line normal to a line between points E and F (angle between force F_{E1} and ground 130)

[0070] β_2 : the angle between ground 130 and a line normal to exoskeleton trunk 109 (angle between force F_{E2} and ground 130)

[0071] α : ground slope (angle between ground 130 and horizontal ground 134)

[0072] D distance between force F_{E2} and point F

[0073] K A constant quantity

[0074] Writing a dynamic equation for the exoskeleton shown in FIG. 5, using equations (1) and (2) and the Lagrangean equation, reveals that the torque provided by right hip actuator 145 between exoskeleton trunk 109 and right leg support 101, T_E , is equal to

$$T_E = (M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + RM_L)g\sin(\beta_1 + \alpha) + T_F + F_{E1}L\cos(\beta_2 - \beta_1) + F_{E2}D \quad (3)$$

where:

[0075] F_{E1} force on exoskeleton trunk 109 from Person's upper body 149, assumed to be normal to the exoskeleton trunk 109 (positive value is shown in FIG. 5)

[0076] F_{E2} force on right leg support 101 from person right lower limb 143, assumed to be normal to a line between points E and F (positive value is shown in FIG. 5)

[0077] T_E : torque generated by right hip actuator 145 (positive value decreases angle λ)

[0078] T_F : friction torque opposing the motion of right leg support 101 relative to exoskeleton trunk 109

Since β_2 is relatively constant in comparison to angle λ (exoskeleton trunk 109 does not rotate much) any interaction torque between person's upper body 149 and exoskeleton trunk 109 will not appear in equation (3). Only the interaction force (e.g., F_{E1} from person's upper body 149 onto exoskeleton trunk 109) affects the motion of exoskeleton trunk 109.

[0079] Rearranging the terms in equation (3) results in equation (4):

$$F_{E1}L\cos(\beta_2 - \beta_1) + F_{E2}D = T_E - (M_{TRUNK}L^2 + I)\ddot{\beta}_1 + (LM_{TRUNK} + RM_L)g\sin(\beta_1 + \alpha) - T_F \quad (4)$$

Assume for a moment that $F_{E2} = 0$. This assumption is only for the sake of understanding the conditions under which the wearer's energy expenditure is reduced. Later, this assumption will be removed. If $F_{E2} = 0$, equation (4) reduces to equation (5).

$$T_E - (M_{TRUNK}L^2 + I)\ddot{\beta}_1 + F_{E1} = \frac{(LM_{TRUNK} + RM_L)g\sin(\beta_1 + \alpha) - T_F}{L\cos(\beta_2 - \beta_1)} \quad (5)$$

We will consider three cases described below.

Case 1

[0080] As can be examined from equation (5), if the hip actuator torque T_E is such that:

$$T_E > (M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + RM_L)g\sin(\beta_1 + \alpha) + T_F \quad (6)$$

Then $F_{E1} > 0$. This means if the hip actuator torque is chosen such that it is larger than the addition of the inertial torque $(M_{TRUNK}L^2 + I)\ddot{\beta}_1$, gravitational torque, $-(LM_{TRUNK} + RM_L)g\sin(\beta_1 + \alpha)$, and the frictional torque T_F , then the force from person 187 on exoskeleton trunk 109 F_{E1} is positive. This means the force from person 187 on exoskeleton trunk 109 is in the direction shown in FIG. 5 and the force on person 187 is generally along the direction of person's forward velocity direction 162. When the force on person 187 is in the direction along the person's forward velocity direction 162 (as shown in FIG. 5), mechanical power is transferred from lower extremity exoskeleton 100 to person 187. Since the time integral of this mechanical power over the entire stance time is positive, mechanical energy is transferred to person 187. Mechanical energy transferred to person 187 during the stance phase will result in an incremental decrease in the wearer's energy required for locomotion during the stance phase. An incremental decrease in the wearer's energy required for locomotion leads to less oxygen consumption and a lower heart rate. The right hand side of inequality (6) represents the torque required to move exoskeleton trunk 109 and right leg support 101 in the stance phase through the same trajectory when exoskeleton 100 is not worn by person 187.

[0081] The situation of Case 1 (described above) shows that in order to reduce the wearer's energy expenditure while walking (and consequently oxygen consumption and heart rate), the torque profile from the hip actuator, when exoskeleton 100 is worn by person 187, should create a force from exoskeleton trunk 109 onto person's upper body along the person's forward velocity direction 162. This means that to

reduce the wearer's energy expenditure while walking, person 187 should be pushed forwardly by exoskeleton trunk 109. The above Case 1 also indicates that to reduce the wearer's energy expenditure while walking (and consequently oxygen consumption and heart rate), the torque profile from the hip actuator, when exoskeleton 100 is worn by person 187, should be larger than the torque required to move exoskeleton trunk 109 and leg support 101 during stance phase through the same trajectory when not worn by person 187.

Case 2

[0082] As can be examined from equation (5), if the hip actuator torque, T_E , is such that:

$$\frac{T_E}{T_F} < (M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha) + \quad (7)$$

then $F_{E1} < 0$. This means that if the hip actuator torque is chosen so that it is smaller than the addition of the inertial torque $(M_{TRUNK}L^2 + I)\ddot{\beta}_1$, gravitational torque, $-(LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha)$ and the frictional torque T_F , then the force on the exoskeleton, F_{E1} , is negative. This means the force from person 187 on exoskeleton trunk 109 is in the opposite direction shown in FIG. 5 and the force on person 187 is along the opposite direction of person's forward velocity direction 162. When the force on person 187 is in the opposite direction of the person's forward velocity direction 162, power is transferred from person 187 to lower extremity exoskeleton 100. Since the time integral of this mechanical power over the entire stance time is negative, mechanical energy is transferred from person 187 to lower extremity exoskeleton 100. Mechanical energy transferred from person 187 during the stance phase will result in an incremental increase in wearer's energy required for locomotion during the stance phase. An incremental increase in wearer's energy required for locomotion leads to more oxygen consumption and higher heart rate for the wearer. The right hand side of inequality (7) represents the torque required to move exoskeleton trunk 109 and right leg support 101 during the stance phase through the same trajectory when not worn by person 187.

Case 3

[0083]

$$\text{If } T_E = (M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + DM_L)g \sin(\beta_1 + \alpha) + T_F \quad (8)$$

Then $F_{E1} = 0$. This means if the hip actuator torque is chosen to be exactly equal to the summation of the inertial torque $(M_{TRUNK}L^2 + I)\ddot{\beta}_1$, gravitational torque, $-(LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha)$, and the frictional torque T_F , then the interaction force between person 187 and the exoskeleton, F_E is zero. This means the person does not feel the exoskeleton and therefore the power person 187 is spending is the same as what he/she would be spending when walking without any exoskeleton. This means no energy is transferred between the exoskeleton and its wearer. In this case, the wearer's energy expenditure neither increases nor decreases.

[0084] If $F_{E2} \neq 0$, the left side of equation (9) represents the torque from person 187 onto lower extremity exoskeleton 100 about point F:

$$F_{E1}L \cos(\beta_2 - \beta_1) + F_{E2}D = T_E - (M_{TRUNK}L^2 + I)\ddot{\beta}_1 + (LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha) - T_F \quad (9)$$

[0085] The three cases described previously for equation (5) can be repeated for equation (9) as described below.

Case 1

[0086] As can be examined from equation (9) if hip actuator torque T_E is such that:

$$\frac{T_E}{T_F} > (M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha) + \quad (10)$$

Then $F_{E1}L \cos(\beta_2 - \beta_1) + F_{E2}D > 0$. This means if the actuator torque is chosen such that it is larger than the summation of the inertial torque $(M_{TRUNK}L^2 + I)\ddot{\beta}_1$, gravitational torque $-(LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha)$, and the frictional torque T_F , then the torque from person 187 onto lower extremity exoskeleton 100 about point F, $F_{E1}L \cos(\beta_2 - \beta_1) + F_{E2}D$, is positive. This means that the torque from person 187 on lower extremity exoskeleton 100 is in the counterclockwise direction and the torque on person 187 is in the clockwise direction and along the person's forward velocity direction 162. When the torque on person 187 is along the person's forward velocity direction 162 (as shown in FIG. 5), power is transferred from lower extremity exoskeleton 100 to person 187. Since the time integral of this power over the entire stance time is positive, mechanical energy is transferred to person 187 from lower extremity exoskeleton 100.

[0087] The situation of Case 1 (described above) teaches that to reduce the wearer's energy expenditure while walking (and consequently oxygen consumption and heart rate), the torque profile from hip actuator when exoskeleton 100 is worn by person 187 should create a clockwise torque from exoskeleton 100 onto person 187 about point F. This means that to reduce the wearer's walking energy expenditure, person 187 should be pushed forwardly by exoskeleton 100. The above Case 1 also teaches that to reduce the wearer's energy expenditure while walking (and consequently oxygen consumption and heart rate), the torque profile from hip actuator when exoskeleton 100 is worn by person 187 should be larger than the torque required to move exoskeleton trunk 109 and leg support in stance phase through the same trajectory when not worn by person 187.

Case 2

[0088] As can be examined from equation (9) if the hip actuator torque, T_E is such that:

$$\frac{T_E}{T_F} < (M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha) + \quad (11)$$

Then $F_{E1}L \cos(\beta_2 - \beta_1) + F_{E2}D < 0$. This means that if the hip actuator torque is chosen such that it is smaller than the summation of the inertial torque $(M_{TRUNK}L^2 + I)\ddot{\beta}_1$, gravitational torque $-(LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha)$, and the frictional torque T_F , then the torque from person 187 onto lower extremity exoskeleton 100 about point F, $F_{E1}L \cos(\beta_2 - \beta_1) + F_{E2}D$, is negative. This means that the torque from person 187 on lower extremity exoskeleton 100 about point F is in the clockwise direction and the torque on person 187 is opposite to the person's forward velocity direction 162 (counterclockwise direction). When the torque on person 187 is opposite to the person's forward velocity direction 162 (as shown in FIG. 5), power is transferred from person 187 to lower extremity exoskeleton 100. If the time integral of this power over the entire stance time is negative, mechanical energy is transferred to lower extremity exoskeleton 100 from person 187.

Case 3

[0089] As can be examined from equation (9), if the hip actuator torque T_E is such that:

$$T_E(M_{TRUNK}L^2+I)\ddot{\beta}_1-(LM_{TRUNK}+RM_L)g\sin(\beta_1+\alpha)+T_F \quad (12)$$

Then $F_{E1} L \cos(\beta_2-\beta_1)+F_{E2} D=0$. This means the torque from person 187 onto lower extremity exoskeleton 100 about point F is zero. If the time integral of this power over the entire stance time is zero, no mechanical energy is transferred between lower extremity exoskeleton 100 and person 187. In this case, the wearer's energy expenditure neither increases nor decreases.

Remark 1

[0090] Since exoskeleton trunk 109 rotates very little (i.e., β_2 is relatively constant in comparison to angle λ) and the summation of torques on exoskeleton trunk 109 is zero, equation (13) states that the torque on exoskeleton trunk 109 from person's upper body cancels the algebraic summation of the reaction torques from hip actuators 145 and 146.

$$T_P=T_E-T_S-T_G \quad (13)$$

where:

[0091] T_P : Torque on exoskeleton trunk 109 from person's upper body 149

[0092] T_E : Torque on exoskeleton trunk 109 from the leg support in stance phase

[0093] T_S : Torque on exoskeleton trunk 109 from the leg support in swing phase (T_S is positive when it tries to turn the exoskeleton trunk in the CW direction around point E)

[0094] T_G : Torque due to the weight of the exoskeleton trunk and any attached load around point E (T_F is positive when it tries to turn the exoskeleton trunk in the CW direction around point E)

[0095] If the leg support that is in the swing phase swings by force of the person, T_S is zero. If the leg support that is in the swing phase swings by power of the hip actuator, T_S is not zero. To reduce T_P (the torque on exoskeleton trunk 109 from person's upper body 149), equation (13) suggests that the leg support in the swing phase be powered (i.e., T_S should be nonzero). This means the hip actuator of the swinging leg should impose a torque in the opposite direction of the hip torque in the stance phase, to reduce the torque the person's upper body 149 supports.

Remark 2

[0096] In general, any lower extremity exoskeleton, regardless of the number of actuators and their locations on the exoskeleton system, decreases its wearer's energy expenditure as long as the force from the exoskeleton trunk onto the wearer's upper body is along the person's forward velocity. For example one can install at least one actuator on each exoskeleton ankle and provide a force from the exoskeleton trunk onto the wearer's upper body along the person's forward velocity. When the force on the person is in the direction along the person's forward velocity, regardless of the exoskeleton architecture, mechanical power is transferred from the exoskeleton to the person. Mechanical energy transferred to the person during the stance phase, will result in an incremental decrease in wearer's energy required for locomotion. An incremental decrease in wearer's energy required for locomotion leads to less oxygen consumption and lower heart rate.

Remark 3

[0097] The above analysis shows how a lower extremity exoskeleton can reduce its wearer's energy expenditure during the stance phase. An exoskeleton system that has two arms, in addition to two lower extremities, can also reduce its wearer's energy expenditure as long as the lower extremities of the exoskeleton function according to the teaching described above.

[0098] In some embodiments, hip actuators 145 and 146 each comprise a hydraulic hip actuator. In these embodiments, at least one power unit 201 provides hydraulic power to hip actuators 145 and 146. In some embodiments, only one power unit 201 provides hydraulic power to hydraulic hip actuators 145 and 146. In some embodiments, each hydraulic hip actuator receives hydraulic power from separate power units. In some embodiments, power unit 201, as shown in FIG. 6, among other components, comprises at least one hydraulic circuit 194 connectable to at least one of hydraulic hip actuators 145 and 146, and modulates the hydraulic fluid flow to and from hydraulic hip actuators 145 and 146. In some embodiments, hydraulic hip actuators 145 and 146 are hydraulic piston-cylinders. In some embodiments, hydraulic hip actuators 145 and 146 are rotary hydraulic vane type hydraulic actuators. In some embodiments, as shown in FIG. 6, hydraulic circuit 194, among other components, comprises a hydraulic pump 240 coupled to an electric motor 241.

[0099] By controlling electric motor 241, a torque profile can be implemented on hip actuators 145, 146 to satisfy the inequalities (6) or (10). Since the torque is a function of the hydraulic pressure and the hip actuator geometry, the hip actuator torque can be controlled by creating a closed loop control on the electric motor 241 by measuring the hydraulic pressure as the feedback variable. In some embodiments, the hip actuator torque can be controlled to satisfy inequalities (6) or (10) by creating a closed loop control on the electric motor 241 by measuring the hip actuator torque or force as the feedback variable.

[0100] In some embodiments, as shown in FIG. 7, hydraulic circuit 194, among other components, further comprises an actuated flow restricting valve 200 capable of redirecting hydraulic fluid from hydraulic right hip actuator 145 around hydraulic pump 240. In operation, when hydraulic pump 240 is in use, actuated flow restricting valve 200 is closed. In operation, when it is necessary to reduce the power consumption, electric motor 241 will not be powered. In that case, actuated flow restricting valve 200 may be opened so that unpowered electric motor 241 and pump 240 will not impede the motion of right hip actuator 145.

[0101] In some embodiments, as shown in FIG. 8, hydraulic circuit 194, among other components, further comprises a three-way valve 242. In operation, while power unit 201 provides hydraulic power to right hip actuator 145, three-way valve 242 connects hydraulic right hip actuator 145 to hydraulic pump 240. In operation, when it is necessary to reduce the power consumption, electric motor 241 will not be powered. In that case three-way valve 242 may redirect hydraulic fluid from hydraulic right hip actuator 145 around hydraulic pump 240 so that unpowered electric motor 241 and pump 240 will not impede the motion of right hip actuator 145.

[0102] FIGS. 6, 7, and 8 show only those components that are needed to accomplish the described task associated with reducing the wearer's energy expenditure. An ordinary

skilled in the art can realize that a hydraulic circuit usually has many other components associated with safety and other features not discussed here.

[0103] Hydraulic hip actuators **145** and **146** comprise any hydraulic actuators or combination of actuators capable of converting pressurized hydraulic fluid into force or torque. Examples of hydraulic actuators include, without limitation, linear hydraulic piston-cylinders, rotary hydraulic actuators, rack-and-pinion-type rotary actuators and rotary hydraulic vane type actuators where pressurized hydraulic fluid, by pushing against moving surfaces, generate force or torque.

[0104] Actuated flow restricting valve **200** comprises any valve or combination of valves capable of performing the indicated functions. Examples of actuated flow restricting valve **200** include, without limitation, flow control valve, pressure control valve, actuated needle valves, solenoid valves and on-off valves. Hydraulic pump **240** comprises any pump or combination of pumps capable of performing the indicated functions. Examples of hydraulic pump **240** include, without limitation gear pump, vane pump, axial piston pump, and radial piston pump.

[0105] Electric motor **241** comprises any device or combination of devices capable of driving hydraulic pump **240**. Examples of motor **241** include, without limitation, electric motors, including, without limitation, AC (alternating current) motors, brush-type DC (direct current) motors, brushless DC motors, electronically commutated motors (ECMs), stepping motors, and any combination thereof. Although we state that electric motor **241** turns hydraulic pump **240**, one skilled in the field can realize that both motor **241** and hydraulic pump **240** may have other types of non-rotational couplings, such as reciprocating linear motion.

[0106] In some embodiments of the invention, lower extremity exoskeleton **100** comprises at least one signal processor **159** capable of controlling hip actuators **145** and **146**. Signal processor **159** comprises an element or combination of elements selected from a group consisting of analog devices; analog computation modules; digital devices including, without limitation, small-, medium-, and large-scale integrated circuits, application specific integrated circuits, programmable gate arrays, programmable logic arrays; electromechanical relays, solid state switches, MOSFET switches and digital computation modules including, without limitation, microcomputers, microprocessors, microcontrollers, and programmable logic controllers. In operation, to decrease the wearer's energy expenditure, signal processor **159** computes a torque profile that satisfies inequalities (6) or (10). This torque is then produced by hip actuators **145** and **146** during their respective stance phase.

[0107] In some embodiments where hip actuators **145** and **146** are hydraulic actuators, signal processor **159**, by controlling electric motor **241**, computes a torque profile as described in inequalities (6) or (10) for hip actuators **145** and **146**. Since the torque is a function of the hydraulic pressure and the hip actuator geometry, the hip actuator torque in some embodiments, as shown in FIG. 8, can be controlled by creating a closed loop control on the electric motor **241** by measuring the hydraulic pressure as the feedback variable. Pressure sensor **236** measures the pressure of the hydraulic fluid and signal processor **159** ensures the pressure is regulated to the desired value. In some embodiments, the hip actuator torque can be controlled to satisfy inequalities (6) or (10) by creating a closed loop control on the electric motor **241** by measuring the hip actuator torque or force as the

feedback variable. A skilled control engineer will be able to develop a controller as shown in FIG. 44 to satisfy inequalities (6) or (10).

[0108] Signal processor **159**, in some embodiments, is mounted to exoskeleton trunk **109**. In some embodiments, signal processor **159** is located inside power unit **201**. Signal processor **159** may be a simple mechanical device consisting of a hydraulic or pneumatic circuit, or it may include electronic elements as well.

[0109] FIG. 5 shows that in order to reduce a wearer's energy expenditure, the force on person **187** should be along the person's forward velocity direction **162**. This can be done either in a closed loop fashion or in an open loop fashion. In the closed loop fashion, one can develop a control algorithm in signal processor **159** to ensure that a force is always imposed on person **187** along the person's forward velocity direction **162**. In some embodiments, this can be done by creating a closed loop force controller on person **187**. The closed loop controller measures the force between person's upper body and exoskeleton **100** and creates a torque for the hip actuator in the stance phase to ensure that this force on the person is always pushing the person forward. In some embodiments, the force between upper body interface device **150** and human upper body is measured as a feedback variable and controlled to be along the person's forward velocity direction **162**. FIG. 44 shows an embodiment of the control block diagram where the force on the wearer's upper body is measured and compared with a desired force onto the wearer's upper body. To reduce the wearer's energy expenditure, this closed loop controller ensures that the force on the wearer's upper body follows the desired force along the wearer's forward velocity. This means that, to reduce the wearer's energy expenditure, the controller ensures the wearer's upper body is pushed forwardly.

[0110] In some embodiments, as shown in FIG. 9, lower extremity exoskeleton **100** comprises at least one stance sensor per leg support, which produces a stance signal indicating whether or not the leg support is in the stance phase. In the embodiment of FIG. 9, leg support **101** includes stance sensor **160**, which produces a stance signal **219**. Stance signal **219** indicates whether leg support **101** is in the stance phase. Similarly, leg support **102** includes stance sensor **161**, which produces a stance signal **220**. Stance signal **220** indicates whether leg support **102** is in the stance phase. In some embodiments, stance sensors **160** and **161** are coupled to supports **101** and **102**, respectively. In operation, signal processor **159** computes a torque profile according to inequalities (6) or (10), depending on whether stance signals **219** and **220** indicate if leg supports **101** and **102** are in either the stance phase or in the swing phase. In some embodiments, stance sensors **160** and **161** are located inside or within the soles of the human shoes (or boots). In some embodiments, stance sensors **160** and **161** are located inside the human shoe or boots. In some embodiments stance sensors **160** and **161** are connectable to the bottom of the human shoes or boots.

[0111] Further discussing the geometry of the exoskeleton shown in FIG. 1, in some embodiments, as shown in FIG. 1, exoskeleton trunk **109**, in addition to other components, comprises two hip links, **114** and **115**, rotatably connectable to thigh links **103** and **104** at hip flexion-extension joints **125** and **126**, allowing for the flexion and extension of leg supports **101** and **102** about hip flexion-extension axes **151** and **152** respectively. In some embodiments, hip links **114** and **115** are rotatably connected to each other at hip abduction-

adduction joint **113**, allowing for abduction and/or adduction of leg supports **101** and **102**. Abduction and adduction of leg supports **101** and **102** are shown by arrows **217** and **218**, respectively.

[0112] FIG. **10** shows another embodiment of the invention where exoskeleton trunk **109** further comprises a hip resilient element **116** configured to apply a torque between hip links **114** and **115**. Examples of a hip resilient element include, without limitation, extension spring, compression spring, leaf spring, gas spring, air spring, rubber, elastomer, surgical tube, bungee cord or combinations thereof. The stiffness of hip resilient element **116** may be chosen such that its force generally holds up the weight of the leg supports **101** or **102** during swing phase.

[0113] In some embodiments, exoskeleton trunk **109** is configured to hold a rear load **118** behind person **187**. FIG. **11** is a perspective drawing wherein exoskeleton trunk **109**, among other components, further comprises a connecting bracket **117** configured to transfer the weight of a rear load **118** to exoskeleton trunk **109**. In some embodiments, as shown in FIG. **12**, connecting bracket **117** further comprises extension frames **119** and **120** configured to hold front load **154** in front of person **187**. Examples of rear load **118** and front load **154** include without limitation, backpacks, baby carriers, food containers, sacks, boxes, water jugs, tool boxes, barrels, ammunition, weaponry, bedding, first aid supplies, golf bags, mail bags, cameras, steady cams, leaf blowers, compressors, electromechanical machineries and combinations thereof. In some embodiments, rear load **118** and/or front load **154** are another person being carried by person **187**. In some embodiments, exoskeleton trunk **109** supports a portion of the weight of person **187** through human upper body interface device **150**.

[0114] Some embodiments, as shown in FIG. **13**, may also include a hip abduction stop **211** which limits or prevents hip links **114** and **115** from abducting with respect to each other. In the particular embodiment shown in FIG. **13**, hip abduction stop **211** is created using a wire rope. Wire rope hip abduction stop **211** prevents abduction of leg supports **101** and **102** past some angle from occurring but allows adduction of leg supports **101** and **102**.

[0115] In accordance with another embodiment of the invention, FIG. **14** is a perspective drawing where exoskeleton trunk **109** includes two hip links **114** and **115** rotatably connectable to thigh links **103** and **104**, allowing for flexion and extension of leg supports **101** and **102** relative to exoskeleton trunk **109**, wherein hip links **114** and **115** are compliantly connected to each other, allowing for abduction and/or adduction of leg supports **101** and **102**. In the example shown in FIG. **14**, this is accomplished by a leaf spring acting as hip resilient element **153**.

[0116] In accordance with another embodiment of the invention, FIG. **15** is a perspective drawing wherein exoskeleton trunk **109**, among other components, further comprises a connecting bracket **117** configured to transfer the weight of a rear load **118** to exoskeleton trunk **109**. Exoskeleton trunk **109** further comprises two hip links **114** and **115** rotatably connectable to thigh links **103** and **104**, allowing for flexion and extension of leg supports **101** and **102** relative to exoskeleton trunk **109**. Hip links **114** and **115** are rotatably connected to connecting bracket **117** via two hip abduction-adduction joints **176** and **177**, and rotate about two hip abduction-adduction axes **178** and **179**. In some embodiments, hip abduction-adduction axes **178** and **179** are gener-

ally parallel to each other. In some embodiments, hip abduction-adduction joints **176** and **177** coincide with each other. Furthermore, in some embodiments, as shown in FIG. **9** through **12**, hip abduction-adduction joints **176** and **177** coincide with each other, forming hip abduction-adduction joint **113**, and hip abduction-adduction axes **178** and **179** become one hip abduction-adduction axis **112**.

[0117] In some embodiments, as shown in FIG. **16**, exoskeleton trunk **109** further comprises abduction-adduction hip resilient elements **121** and **122**, configured to apply torques between hip links **114** and **115** and connecting bracket **117**. Examples of hip abduction-adduction resilient elements include, without limitation, extension spring, compression spring, gas spring, air spring, rubber, surgical tube, leaf springs, bungee cord and combinations thereof. The stiffness of abduction-adduction hip resilient elements **121** and **122** may be chosen such that its force generally holds up the weight of the leg supports **101** or **102** during swing phase and aid the person in keeping the load oriented vertically while walking.

[0118] In some embodiments, as shown in FIG. **17**, hip links **114** and **115** are compliantly connected to connecting bracket **117**. In the embodiment shown in FIG. **17**, this is accomplished by a hip resilient element **153**, which in this case is a leaf spring. In some embodiments, as shown in FIG. **17**, exoskeleton trunk **109** comprises a backpack frame **180** that allows a backpack to be coupled to lower extremity exoskeleton **100**. In some embodiments, backpack frame **180** is connected to connecting bracket **117**. The upper body interface devices **150** (such as a belt and shoulder straps) have been omitted in this figure for clarity; however, upper body interface devices **150**, in some embodiments, can be coupled to backpack frame **180** or connecting bracket **117**.

[0119] In accordance with another embodiment, FIG. **18** is a perspective drawing wherein leg supports **101** and **102** further include thigh abduction-adduction joints **123** and **124**, which are configured to allow abduction and/or adduction of leg supports **101** and **102** about thigh abduction-adduction axes **202** and **203**, respectively. In some embodiments, thigh abduction-adduction joints **123** and **124** are located below hip flexion-extension joints **125** and **126**. These joints are shown in greater detail in FIG. **19**, which is a partial view of the same embodiment of FIG. **18**.

[0120] In some embodiments, as shown in FIG. **19**, right leg support **101** includes a thigh adduction stop **185**, which limits or prevents right thigh link **103** from adducting at thigh abduction-adduction joints **123** and **124**. Abduction and adduction of right leg support **101** are shown by arrows **227** and **228**, respectively. In the particular embodiment shown in FIG. **19**, right thigh abduction-adduction joint **123** includes a thigh adduction stop **185**, which bears on a thigh stop surface **186**. Thigh adduction stop **185** limits the adduction of thigh abduction-adduction joint **123**. The unrestricted adduction of right thigh abduction-adduction joint **123**, during stance phase, would cause right hip link **114** to move downwardly along arrow **204** during stance phase, thereby dropping (lowering) the load. Such abduction-only joints for thigh abduction-adduction joints **123** and **124** are useful in allowing the person to squat naturally. In some embodiments, like the one shown in FIGS. **18** and **19**, such abduction joints are generally located below hip flexion-extension joints **125** and **126**.

[0121] In some embodiments, as shown in FIGS. **18** and **19**, leg supports **101** and **102** further include leg rotation joints **127** and **128** configured to allow rotation of leg supports **101**

and 102. Leg rotation joints 127 and 128 are generally located above knee joints 107 and 108. Lines 164 and 165 represent the leg rotation axes of leg rotation joints 127 and 128. In FIGS. 19 and 20, this is accomplished by providing for a sliding contact between the right hip rotation shaft 166 and the right hip rotation journal 168. The parts included in the joint which prevent it from pulling apart have been omitted for simplicity, but one skilled in the art will note that there are many ways of retaining such shafts in such journals.

[0122] In some embodiments, as shown in FIG. 20, leg rotation joints 127 and 128 further comprise a rotation resilient element 129. This rotation resilient element acts as a torsion spring and provides a restoring torque, which generally restores the leg support back to the neutral position shown in FIG. 18 from an extended position (not shown). Rotation resilient element 129 can be constructed in many ways, with the particular cross section shown in FIG. 20 being advantageous when using an elastomeric material to construct the element. Rotation resilient element 129 is shown partially deflected for illustration purposes.

[0123] Also, in some embodiments, as shown in FIG. 19 and FIG. 20, leg supports 101 and 102 further comprise compression-elongation mechanisms 131 and 132, configured to change the distance between exoskeleton trunk 109 and the respective knee flexion-extension joints 107 and 108. In some embodiments, compression-elongation mechanisms 131 and 132 allow for changes in the distance between the hip flexion-extension joints 125 and 126 and the respective flexion-extension knee joints 107 and 108. The compression-elongation mechanisms contract by right hip rotation shaft 166 sliding further into the right hip rotation journal 168 (shown for right leg 101 only). The leg rotation resilient element 129 is allowed to slide into a clearance cavity 170. In some embodiments, compression-elongation mechanism 131 and 132 further comprise a right leg compression-elongation resilient element 133. This leg compression-elongation resilient element acts as a spring and provides a restoring force, which generally restores the leg support back to a neutral configuration from an extended configuration. In the embodiment of FIG. 20, this is illustrated by a helical compression spring.

[0124] In some embodiments, as shown in FIG. 18, exoskeleton hip mechanism cover 171 may cover some components of exoskeleton, including parts of hip links 114 and 115, hip resilient element 116 or abduction-adduction hip resilient elements 121 and 122. In some embodiments, as shown in FIG. 18, leg supports 101 and 102 further comprise exoskeleton feet 139 and 140, coupled to shank links 105 and 106, respectively, allowing the transfer of forces from shank links 105 and 106 to the ground. In operation, exoskeleton feet 139 and 140 are configurable to be coupled to the feet of person 187. In some embodiments, as shown in FIG. 18, the coupling to person's feet is accomplished by using clam-shell type bindings 205 and 206, as sometimes found on modern snow shoes. However, there are a great number of methods to make such a connection, as can be seen on different types of snow skis, snowboards, snowshoes and other such devices. In some embodiments, as shown in FIG. 21, exoskeleton feet 139 and 140 comprise exoskeleton shoes 188 and 189, wearable by person 187, thereby allowing exoskeleton feet 139 and 140 to couple to the feet of person 187. In some embodiments, as shown in FIG. 22, exoskeleton feet 139 and 140 comprise exoskeleton insoles 157 and 158, insertable inside the person's shoes, allowing exoskeleton feet 139 and 140 to couple

to the feet of person 187. Insoles 157 and 158 are flexible and therefore can bend to match the curvature of the human foot during maneuvers such as squatting. Also, the insole side supports 212 are either compliant or configured to include degrees of freedom to mimic the movement of the human ankle.

[0125] In some embodiments, as shown in FIG. 18, exoskeleton feet 139 and 140 are compliantly coupled to shank links 105 and 106. This is accomplished using ankle resilient elements 181 and 182. FIG. 23 shows a close-up view of right exoskeleton foot 139. In this example, right ankle resilient element 181 is constructed of a metal ball-and-socket joint 231 surrounded by a doughnut shaped elastomer element 230, which creates compliance in all directions of rotations.

[0126] In some embodiments, exoskeleton feet 139 and 140 rotate about two plantar-dorsi flexion axes relative to shank links 105 and 106. FIG. 24 shows an embodiment of this type of exoskeleton where right ankle plantar-dorsi flexion axis 172 is generally parallel to the plantar-dorsi flexion axis in the human ankle. In some embodiments, each leg support further comprises at least one ankle plantar-dorsi flexion resilient element 141 resisting the rotation of respective exoskeleton foot about right ankle plantar-dorsi flexion axis 172.

[0127] In some embodiments, exoskeleton feet 139 and 140 rotate about two ankle abduction-adduction axes relative to shank links 105 and 106. FIG. 25 shows an embodiment of this type of exoskeleton where right ankle abduction-adduction axis 174 is generally parallel to the abduction-adduction axis in the human ankle. In some embodiments, each leg support further comprises at least one ankle abduction-adduction resilient element 142 resisting the rotation of right exoskeleton foot 139 about right ankle abduction-adduction axis 174, as depicted in FIG. 25.

[0128] In some embodiments, exoskeleton feet 139 and 140 rotate about an ankle rotation axes 147 relative to shank links 105 and 106. In some embodiments, as shown in FIG. 26, this is accomplished using a shank rotation joint 207, which functions similar to leg rotation joint 127. FIG. 26 shows an embodiment of this type of exoskeleton where right ankle rotation axis 147 is generally parallel to the rotation axis in the human ankle. In some embodiments, resilient elements can be included in the ankle to resist the rotation of right exoskeleton foot 139 about right ankle rotation axis 147.

[0129] FIG. 27 shows an embodiment of the embodiment of FIG. 5 where right exoskeleton foot 139 has been added. The analysis described above on the power transfer between person 187 and lower extremity exoskeleton 100 applies to the exoskeleton in FIG. 27, if one assumes the rotation of right leg support 101 about point F in FIG. 5 occurs at right ankle point 155.

[0130] In some embodiments, as shown in FIG. 28, stance sensors 160 and 161 are integrated into exoskeleton feet 139 and 140. In some embodiments, as shown in FIG. 28, stance sensor 160 is a pressure sensor measuring the pressure in a media 191 trapped in a stance sensor cavity 192 inside right exoskeleton foot 139. FIG. 23 shows an embodiment where a tube is used as a stance sensor cavity 192. In some cases, the stance signals 219 and 220 may take the form of the media 191 itself transported in a small tube from stance sensor cavity 192 to signal processor 159.

[0131] FIG. 29 shows another embodiment wherein stance sensor 160 is a force sensor connectable to right exoskeleton foot 139. In some embodiments, as shown in FIG. 30, stance sensor 160 is located inside the human shoe like an insole and

its output signal represents the force on the bottom of the human foot. This type would be particularly useful in embodiments of the invention such as those shown in FIG. 21 or 22. In some embodiments, as shown in FIG. 31, stance sensor 160 is connected to the bottom of the human shoe and senses the force on the bottom of the human foot. In some embodiments, as shown in FIG. 32, stance sensor 160 is located inside the human shoe sole and senses the force on the bottom of the human foot. In some embodiments, stance sensors 160 and 161 are coupled to shank links 105 and 106, respectively. Stance sensor 160 comprises any sensor or combination of sensors capable of performing the indicated functions. Examples of stance sensor 160 include, without limitation, force sensors, strain-gage based force sensors, piezoelectric force sensors, force sensing resistors, pressure sensors, switches, tape switches and combinations thereof. In some embodiments stance sensor 160 is a switch that represents the existence of a force greater than some threshold force on the bottom of the foot of person 187.

[0132] Also shown in FIG. 33 is an additional thigh abduction-adduction joint 235, which is included in order to allow the leg to be stowed in a vertical position when the exoskeleton is not in use but needs to be carried. Right leg support 101 can abduct along an additional right thigh abduction-adduction axis 237 (depicted in FIG. 34). This may be desirable if person 187 no longer has a very heavy load to carry but needs to transport lower extremity exoskeleton 100. In that case, the operator may unstrap the exoskeleton's right leg support 101 and swing the leg outward from his or her body until the right exoskeleton foot 139 is in the air over the operator's head. Then, by bending the right knee joint 107 and/or rotating the right leg rotation joint 127, the leg can be positioned such that it stows behind the operator, as shown in FIG. 33. This is possible because the right thigh abduction-adduction joint 123 and the additional right thigh abduction-adduction joint 235 each allow for a rotation of approximately ninety degrees about the right thigh abduction-adduction axis 202 and the additional right thigh abduction-adduction axis 237, respectively. The total abduction therefore possible is over 180 degrees. This could be accomplished with one thigh abduction-adduction joint which has 180 degrees of travel, but designing such a joint would cause the designer to move the pivot point of the joint outward from the operator a great deal, which would result in a wider exoskeleton design. This is undesirable but is a viable alternative design.

[0133] In some embodiments, lower extremity exoskeleton 100 (as shown in FIG. 1) comprises two torque generators 110 and 111, which are configured to allow flexion of knee joints 107 and 108 during swing phase and resist flexion of knee joints 107 and 108 during stance phase, thereby allowing the lower extremity exoskeleton 100 to bear a load and transfer the load forces (e.g., load weight) to the ground. In some embodiments, torque generators 110 and 111 are hydraulic torque generators. In accordance with some embodiments, torque generators 110 and 111 are hydraulic piston cylinders where the motion of the piston relative to the cylinder creates hydraulic fluid flow into or out of the cylinder. In operation, the hydraulic fluid flow into or out of the cylinder may be controlled by a hydraulic valve. The smaller the hydraulic valve orifice size is, the more force is needed to move the piston relative to the cylinder with a given speed. In other words, the more damped the motion of the piston relative to the cylinder needs to be, the smaller the hydraulic valve orifice size should be. If the hydraulic valve orifice size is

large, then a small force is required to move the piston relative to the cylinder. Here, impedance of hydraulic torque generators 110 and 111 is defined as the ratio of the required force over the velocity in frequency domain. With this definition, the smaller the hydraulic valve orifice size is, the larger the impedance of the hydraulic torque generator will be.

[0134] In some embodiments, as shown in FIG. 35, torque generators 110 and 111 are hydraulic rotary dampers where the torque produced may be controlled by a hydraulic valve. The smaller the hydraulic valve orifice size is, the more torque is needed to rotate the hydraulic rotary damper with a given speed. In other words, the more damped the rotation of the hydraulic rotary damper needs to be, the smaller the hydraulic valve orifice size should be. Here impedance of hydraulic rotary dampers 110 and 111 is defined as the ratio of the required torque over the angular velocity in frequency domain. With this definition, the smaller the hydraulic valve orifice size is, the larger the impedance of the hydraulic rotary damper will be.

[0135] In some embodiments, torque generators 110 and 111 are friction brakes where one can control the resistive torque on knee joints 107 and 108 by controlling the friction torques. In other embodiments, torque generators 110 and 111 are viscosity based friction brakes where one can control the resistive torque on knee joints 107 and 108 by controlling the viscosity of the fluid. In other embodiments, torque generators 110 and 111 are Magnetorheological Fluid Devices where one can control the resistive torque on knee joints 107 and 108 by controlling the viscosity of the Magnetorheological Fluid. One skilled in the art realizes that any of the above devices can be mounted in the invention to function in the same way as the hydraulic rotary dampers shown in FIG. 35.

[0136] In some embodiments, signal processor 159 is configured to control torque generators 110 and 111. Signal processor 159 controls the resistance to flexion in knee joints 107 and 108 as a function of stance signals 219 and 220. For example, when right stance sensor 160 detects the stance phase in right leg support 101, signal processor 159 will increase the impedance of right torque generator 110 so that right knee joint 107 resists flexion. Conversely, when right stance sensor 160 detects the swing phase in right leg support 101, signal processor 159 will decrease the impedance of right torque generator 110 so that no resistance to flexion occurs in right knee joint 107. Similarly, when stance sensor 161 detects the stance phase in left leg support 102, signal processor 159 will increase the impedance of left torque generator 111 so that left knee joint 108 resists flexion. Conversely, when left stance sensor 161 detects the swing phase in left leg support 102, signal processor 159 will decrease the impedance of left torque generator 111 so that no resistance to flexion occurs in left knee joint 108. Large impedances of torque generators 110 and 111 lead to large resistance of knee joints 107 and 108 to flexion needed during stance phase. Conversely, small impedances of torque generators 110 and 111 lead to small resistance of knee joints 107 and 108 to flexion needed during swing phase. In some embodiments, signal processor 159 is mounted to torque generators 110 and 111.

[0137] In practice, the resistance to flexion in knee joints 107 and 108 during the stance phase need not be constant. In some embodiments, the resistance to flexion at the beginning of the stance phase (approximately the first 20% of the stance cycle) may be extremely high (i.e., knee joints 107 and 108 will be locked in the beginning of stance). During the middle

of the stance phase (approximately the 20% to 80% of the stance cycle), the resistance to flexion may be lower, but high enough that knee joints **107** and **108** will only undergo a few degrees of flexion. During the end of the stance cycle (approximately the last 20% of the stance cycle), the resistance to flexion may be low, but still nonzero, so that knee joint **107** and **108** may flex in preparation for the swing cycle.

[0138] In some embodiments, each of leg supports **101** and **102** further comprises a torque generator wherein each torque generator comprises a hydraulic piston-cylinder. In these embodiments, power unit **201**, among other components, comprises at least one knee hydraulic circuit **190** connectable to torque generators **110** and **111**. Knee hydraulic circuit **190** is configured to modulate the fluid flow to torque generators **110** and **111**. In operation (using right leg support **101** as an example), when right leg support **101** is in a stance phase, knee hydraulic circuit **190** is configured to restrict the fluid flow to right torque generator **110** of right leg support **101**. Knee hydraulic circuit **190**, when leg support **101** is in a swing phase, is configured to allow the fluid flow to right torque generator **110** of right leg support **101**. In other words, knee hydraulic circuit **190**, when leg support **101** is in a stance phase, is configured to increase the resistance to flexion of right knee joint **107**. Knee hydraulic circuit **190**, when leg support **101** is in a swing phase, is configured to decrease the resistance to flexion of right knee joint **107**. The above behavior is also true for leg support **102**. In some embodiments of the invention, lower extremity exoskeleton **100** further comprises at least one stance sensor **160** and **161** for each of leg supports **101** and **102**. Stance sensors **160** and **161** produce stance signals **219** and **220**, indicating whether leg supports **101** and **102** are in the stance phase. In some embodiments, knee hydraulic circuit **190** and hydraulic circuit **194** may be coupled to each other or share components. In some embodiments, one knee hydraulic circuit **190** may be used for both torque generator **110** and **111**, or each of torque generators **110** and **111** may connect to an independent knee hydraulic circuit **190**.

[0139] FIG. 36 shows an embodiment of the invention where knee hydraulic circuit **190** comprises a knee actuated flow-restricting valve **208** connecting right torque generator **110** to a hydraulic reservoir **195**. In operation, knee actuated flow-restricting valve **208** restricts the fluid flow during stance phase and allows for minimum resistance fluid flow during the swing phase. Although one reservoir (i.e., reservoir **195**) is used to hold hydraulic fluid for both hydraulic circuit **194** and knee hydraulic circuit **190**, one can use separate hydraulic reservoirs for hydraulic circuit **194** and knee hydraulic circuit **190**.

[0140] FIG. 37 shows an embodiment of the invention where knee hydraulic circuit **190** comprises a hydraulic three-way valve **198** connecting right torque generator **110** to a hydraulic reservoir **195**, either through a non-actuated flow restricting valve **196** or a bypass line **197**. Hydraulic three-way valve **198** connects right torque generator **110** to hydraulic reservoir **195** through non-actuated flow restricting valve **196** during stance phase, thereby restricting the hydraulic flow and increasing the impedance of right torque generator **110**. During swing phase, hydraulic three-way valve **198** connects right torque generator **110** to hydraulic reservoir **195** through bypass line **197**, thereby increasing the hydraulic fluid flow and decreasing the impedance of right torque generator **110**.

[0141] FIG. 38 represents another embodiment of knee hydraulic circuit **190**, where a knee actuated flow-restricting valve **208** capable of controlling its orifice size and a check valve **199** connect torque generator **110** to hydraulic reservoir **195**. In operation during the stance phase, signal processor **159** restricts the fluid flow by controlling the orifice of knee actuated flow-restricting valve **208**. During swing phase, signal processor **159** opens knee actuated flow-restricting valve **208** and allows for fluid flow to torque generator **110** thereby decreasing the impedance of torque generator **110**. Knee actuated flow-restricting valve **208** comprises any valve or combination of valves capable of performing the indicated functions. Examples of knee actuated flow-restricting valve **208** include, without limitation, flow control valves, pressure control valves and on-off valves. Check valve **199** allows right knee joint **107** to extend easily (no or minimum resistance) at all times.

[0142] FIG. 39 represents another embodiment of knee hydraulic circuit **190**. This embodiment is similar to the embodiment of FIG. 37, but an additional check valve **199** has been added to allow right knee joint **107** to extend easily (no or minimum resistance) at all times.

[0143] FIG. 40 represents another embodiment of knee hydraulic circuit **190** where a two-way valve **193**, capable of selecting between a set orifice size or fully open orifice, and check valve **199** connect torque generator **110** to hydraulic reservoir **195**. During stance phase, signal processor **159** directs the fluid flow to torque generator **110** through the set orifice size of two-way valve **193**. During swing phase, signal processor **159** directs the fluid flow to torque generator **110** through fully open orifice of two-way valve **193**. Check valve **199** allows right knee joint **107** to extend easily (no or minimum resistance) at all times.

[0144] In some embodiments, leg supports **101** and **102** are configured to allow flexion of the respective knee joints **107** and **108** during the swing phase and to resist flexion of the respective knee joints **107** and **108** during the stance phase by locking the knees. One such locking knee is shown in FIG. 41. FIG. 41 shows right leg support **101** in two configurations. In FIG. 41, right shank link **105** includes a shank stop **209**, which bears on thigh stop **210** when the knee is hyperextended. The angle of right knee joint **107** at hyper-extension is illustrated as A in FIG. 41. Since this angle is less than 180 degrees, knee joint **107** or **108** will go “over-center” when approaching hyper-extension, meaning that the knee will tend to lock against the stops if leg supports **101** or **102** are subject to a compressive load, as would be the case for right leg support **101** in the situation illustrated in FIG. 41. One skilled in the art will note that there are many such over-center mechanisms, which generally tend to force the load vector on the leg support to pass in front of the knee joint.

[0145] In some embodiments, lower extremity exoskeleton **100** further comprises knee resilient elements **232**, which are configured to encourage flexion of knee joints **107** and **108**. This decreases the person’s effort needed to flex knee joints **107** and **108** during the swing phase. In some embodiments, as shown in FIG. 42, knee resilient elements **232** are in parallel with torque generators **110** and **111**. In some embodiments, knee resilient elements **232**, as shown in FIG. 43, are in series with torque generators **110** and **111**. In some embodiment, lower extremity exoskeleton **100** comprises knee resilient elements **232**, which are configured to encourage extension of knee joints **107** and **108**. One skilled in the art will note that there are many methods and locations for

installation of knee resilient element **232** to encourage flexion and/or extension of knee joints **107** and **108**. It is further understood that knee resilient elements **232** can also be used with the embodiment of the exoskeleton shown in FIG. **41**.

[0146] Although various exemplary embodiments have been described, it will be appreciated by persons skilled in the art that numerous variations and/or modifications may be made to the described device as specifically shown here without departing from the spirit or scope of that broader disclosure. For example, in general, the exoskeleton legs do not have to reach all the way to the ground in order to decrease the wearer's oxygen consumption. Any leg support including shank links only, as shown in FIG. **45**, decrease its wearer's energy expenditure as long as the force from exoskeleton trunk onto the wearer's upper body is along the person's forward velocity. The mechanical energy transferred to the person during the stance phase will result in an incremental decrease in wearer's energy required for locomotion during the stance phase. An incremental decrease in wearer's energy required for locomotion leads to less oxygen consumption and a lower heart rate. The various examples are, therefore, to be considered in all respects as illustrative and not restrictive. In general, the invention is only intended to be limited by the scope of the following claims.

We claim:

1. A method of reducing energy consumption of a person in motion along a trajectory in a forward direction of movement coupled to an exoskeleton device including at least one power unit, two leg supports for coupling to said person's lower limbs rotatably connected to an exoskeleton trunk, and two hip actuators for creating torques between said leg supports and said exoskeleton trunk, said method comprising: supplying energy from said at least one power unit to said hip actuator of the leg support coupled to said person's lower limb in a stance phase wherein said energy is determined based on a force between said exoskeleton trunk and the person's upper body along the person's forward velocity direction and established to be larger than an amount of energy required to move said exoskeleton trunk and said leg support in the stance phase through the same trajectory in the forward direction of movement when not worn by said person.

2. The method of claim **1**, further comprising: determining said energy to establish a torque profile for controlling said hip actuator of said leg support in the stance phase to ensure said torque profile is larger than:

$$(M_{TRUNK}L^2+I)\ddot{\beta}_1-(LM_{TRUNK}+RM_L)g \sin(\beta_1+\alpha)+T_F$$

wherein:

M_{TRUNK} is a mass of the exoskeleton trunk and any attached load;

M_L is a mass of the respective first and second leg support in the stance phase;

I is moment of inertia of the respective first and second leg support in the stance phase;

L is a length of the respective first and second leg support in the stance phase;

R is a distance between a center of mass of the respective first and second leg support in the stance phase and a rotational point;

g is force due to gravity;

β_1 is an angle between a support surface and the normal line of force on the exoskeleton trunk from the person's upper body;

α is a ground slope defined by an angle between a support surface and a horizontal plane; and

T_F is a frictional torque opposing the motion of the leg support relative to the exoskeleton trunk.

3. The method of claim **1**, wherein supplying energy from said at least one power unit to said hip actuator of the leg support coupled to said person's lower limb in the stance phase includes creating a torque profile in said hip actuator of said leg support in the stance to provide torque at least equal to an amount of torque required to move said exoskeleton trunk and said leg support in the stance phase through the same trajectory in the forward direction of movement when not worn by said person.

4. The method of claim **3**, wherein each said leg support further comprises a thigh link, a shank link, and a knee joint configured to allow flexion and extension between said shank link and said thigh link, said method further comprising: allowing flexion and extension of a respective said knee joint during a swing phase and resisting flexion of the respective said knee joint during the stance phase to allow a transfer of force to the ground.

5. The method of claim **1**, wherein supplying energy from said at least one power unit to said hip actuator of the leg support coupled to said person's lower limb in the stance phase includes creating a force from said exoskeleton trunk onto the person's upper body by use of said hip actuator of said leg support in the stance phase, wherein said force from said exoskeleton trunk onto the person's upper body is along the person's forward velocity.

6. The method of claim **5** further comprising:

measuring the force between said exoskeleton trunk and the person's upper body; and

ensuring that the force from said exoskeleton trunk onto the person's upper body is always along the person's forward velocity.

7. The method of claim **1**, further comprising: transferring weight of a load to said exoskeleton trunk through a connecting bracket.

8. The method of claim **7**, further comprising: holding the load in front of the person through an extension frame when said exoskeleton trunk is coupled to said person's upper body.

9. The method of claim **1**, further comprising: producing a stance signal utilizing at least one stance sensor for each said leg support, with the stance signal indicating whether a respective said leg support is in the stance phase.

10. The method of claim **9**, wherein said at least one stance sensor is located inside or connected to a bottom of a human shoe.

11. The method of claim **1**, wherein each said leg support includes a foot configured to rest on the ground and each said foot includes at least one stance sensor, said method further comprising: producing a stance signal utilizing the at least one stance sensor indicating whether a respective said leg support is in the stance phase.

12. A method of reducing energy consumption of a person in motion along a trajectory in a forward direction of movement coupled to an exoskeleton device including at least one power unit, two leg supports rotatably connected to an exoskeleton trunk for attachment to the person's legs, and two hip actuators for creating torques between said leg supports and said exoskeleton trunk, the method comprising: supplying energy from said at least one power unit to said hip actuator of the leg support coupled to said person's lower limb in a stance phase to create a force from said exoskeleton trunk onto the

person's upper body by use of said hip actuator of said leg support in the stance phase, wherein said force from said exoskeleton trunk onto the person's upper body is along the person's forward velocity and larger than an amount of energy required to move said exoskeleton trunk and said leg support in the stance phase through the same trajectory in the forward direction of movement when the exoskeleton is not worn by said person.

13. The method of claim **12**, further comprising: measuring a force between said exoskeleton trunk and the person's upper body and ensuring that the force from said exoskeleton trunk onto the person's upper body is always along the person's forward velocity.

14. The method of claim **12**, further comprising: transferring weight of a load to said exoskeleton trunk through a connecting bracket.

15. The method of claim **14**, further comprising: holding the load in front of the person through an extension frame when said exoskeleton trunk is coupled to said person's upper body.

16. The method of claim **12**, further comprising: producing a stance signal utilizing at least one stance sensor for each said leg support, with the stance signal indicating whether a respective said leg support is in the stance phase.

17. The method of claim **16**, wherein each said leg support includes a foot configured to rest on the ground, and each said foot includes the at least one stance sensor producing the stance signal.

18. The method of claim **12**, further comprising: determining said energy to establish a torque profile for controlling said hip actuator of said leg support in the stance phase to ensure said torque profile is larger than:

$$(M_{TRUNK}L^2 + I)\ddot{\beta}_1 - (LM_{TRUNK} + RM_L)g \sin(\beta_1 + \alpha) + T_F$$

wherein:

M_{TRUNK} is a mass of the exoskeleton trunk and any attached load;

M_L is a mass of the respective first and second leg support in the stance phase;

I is moment of inertia of the respective first and second leg support in the stance phase;

L is a length of the respective first and second leg support in the stance phase;

R is a distance between a center of mass of the respective first and second leg support in the stance phase and a rotational point;

g is force due to gravity;

β_1 is an angle between a support surface and the normal line of force on the exoskeleton trunk from the person's upper body;

α is a ground slope defined by an angle between a support surface and a horizontal plane; and

T_F is a frictional torque opposing the motion of the leg support relative to the exoskeleton trunk.

19. The method of claim **12**, wherein supplying energy from said at least one power unit to said hip actuator of the leg

support coupled to said person's lower limb in the stance phase includes creating a torque profile in said hip actuator of said leg support in the stance to provide torque at least equal to an amount of torque required to move said exoskeleton trunk and said leg support in the stance phase through the same trajectory in the forward direction of movement when not worn by said person.

20. The method of claim **19**, wherein each said leg support further comprises a thigh link, a shank link, and a knee joint configured to allow flexion and extension between said shank link and said thigh link, said method further comprising: allowing flexion and extension of a respective said knee joint during a swing phase and resisting flexion of the respective said knee joint during the stance phase to allow a transfer of force to the ground.

21. A method of reducing the energy consumption of a person in motion along a direction of movement coupled to an exoskeleton device including at least one power unit, two leg supports for coupling to said person's lower limbs rotatably connected to an exoskeleton trunk, two hip actuators for creating torques between said leg supports and said exoskeleton trunk, and at least one signal processor, said method comprising:

supplying energy from said at least one power unit to said hip actuator of the leg support coupled to said person's lower limb in a stance phase and creating a torque profile for said hip actuator of said leg support in the stance phase such that mechanical energy is transferred to said person from said lower extremity exoskeleton during said stance phase in the direction of movement, wherein said signal processor computes said torque profile and controls said hip actuator of said leg support in the stance phase to ensure said torque profile is larger than the sum of inertial, gravitation and frictional torques on said leg support in the stance phase.

22. A method of reducing energy consumption of a person in motion along a trajectory in a direction of movement coupled to an exoskeleton device including two leg supports for coupling to said person's lower limbs rotatably connected to an exoskeleton trunk, two hip actuators for creating torques between said leg supports and said exoskeleton trunk, at least one power unit for providing power to said hip actuators, and at least one processor wherein, when said lower extremity exoskeleton is worn by the person, one of the two leg supports is in a stance phase and another of the two leg supports is in a swing phase, said method comprises:

creating a torque profile which is larger than a required torque or energy needed to move said exoskeleton trunk and said one of the two leg supports in the stance phase through the same trajectory when not worn by said person; and

causing the hip actuator for said one of the two leg supports which in the stance phase to follow the torque profile.

* * * * *