



US 20230000567A1

(19) **United States**

(12) **Patent Application Publication**

FLEXMAN et al.

(10) **Pub. No.: US 2023/0000567 A1**

(43) **Pub. Date: Jan. 5, 2023**

(54) **DEVICE VISUALIZATION THROUGH OPTICAL SHAPE SENSING OF A GUIDEWIRE**

(71) Applicant: **KONINKLIJKE PHILIPS N.V., EINDHOVEN (NL)**

(72) Inventors: **Molly Lara FLEXMAN, MELROSE, MA (US); Gregory COLE, OSSINING, MA (US); David Paul NOONAN, NEW YORK, NY (US); Neriman Nicoletta KAHYA, EINDHOVEN (NL)**

(21) Appl. No.: **17/903,340**

(22) Filed: **Sep. 6, 2022**

Publication Classification

(51) **Int. Cl.**
A61B 34/20 (2016.01)
A61B 90/00 (2016.01)
A61B 5/00 (2006.01)
A61F 2/07 (2013.01)
A61B 5/107 (2006.01)
A61F 2/95 (2013.01)
A61F 2/06 (2013.01)

(52) **U.S. Cl.**
CPC *A61B 34/20* (2016.02); *A61B 90/39* (2016.02); *A61B 5/6851* (2013.01); *A61F 2/07* (2013.01); *A61B 5/1076* (2013.01); *A61F 2/95* (2013.01); *A61B 5/0084* (2013.01); *A61B 5/6876* (2013.01); *A61B 2090/3966* (2016.02); *A61B 2034/2061* (2016.02); *A61F 2002/065* (2013.01)


Related U.S. Application Data

(63) Continuation of application No. 15/544,925, filed on Jul. 20, 2017, filed as application No. PCT/IB2015/060063 on Dec. 31, 2015.

(60) Provisional application No. 62/106,267, filed on Jan. 22, 2015.

(57) **ABSTRACT**

A medical device deployment system includes a main body and a guidewire capable of being passed through the main body and including a lumen. An optical shape sensing (OSS) system is configured to pass through the lumen in the guidewire. The OSS system is configured to measure shape, position or orientation of an endograft relative to a blood vessel for placement of the endograft.

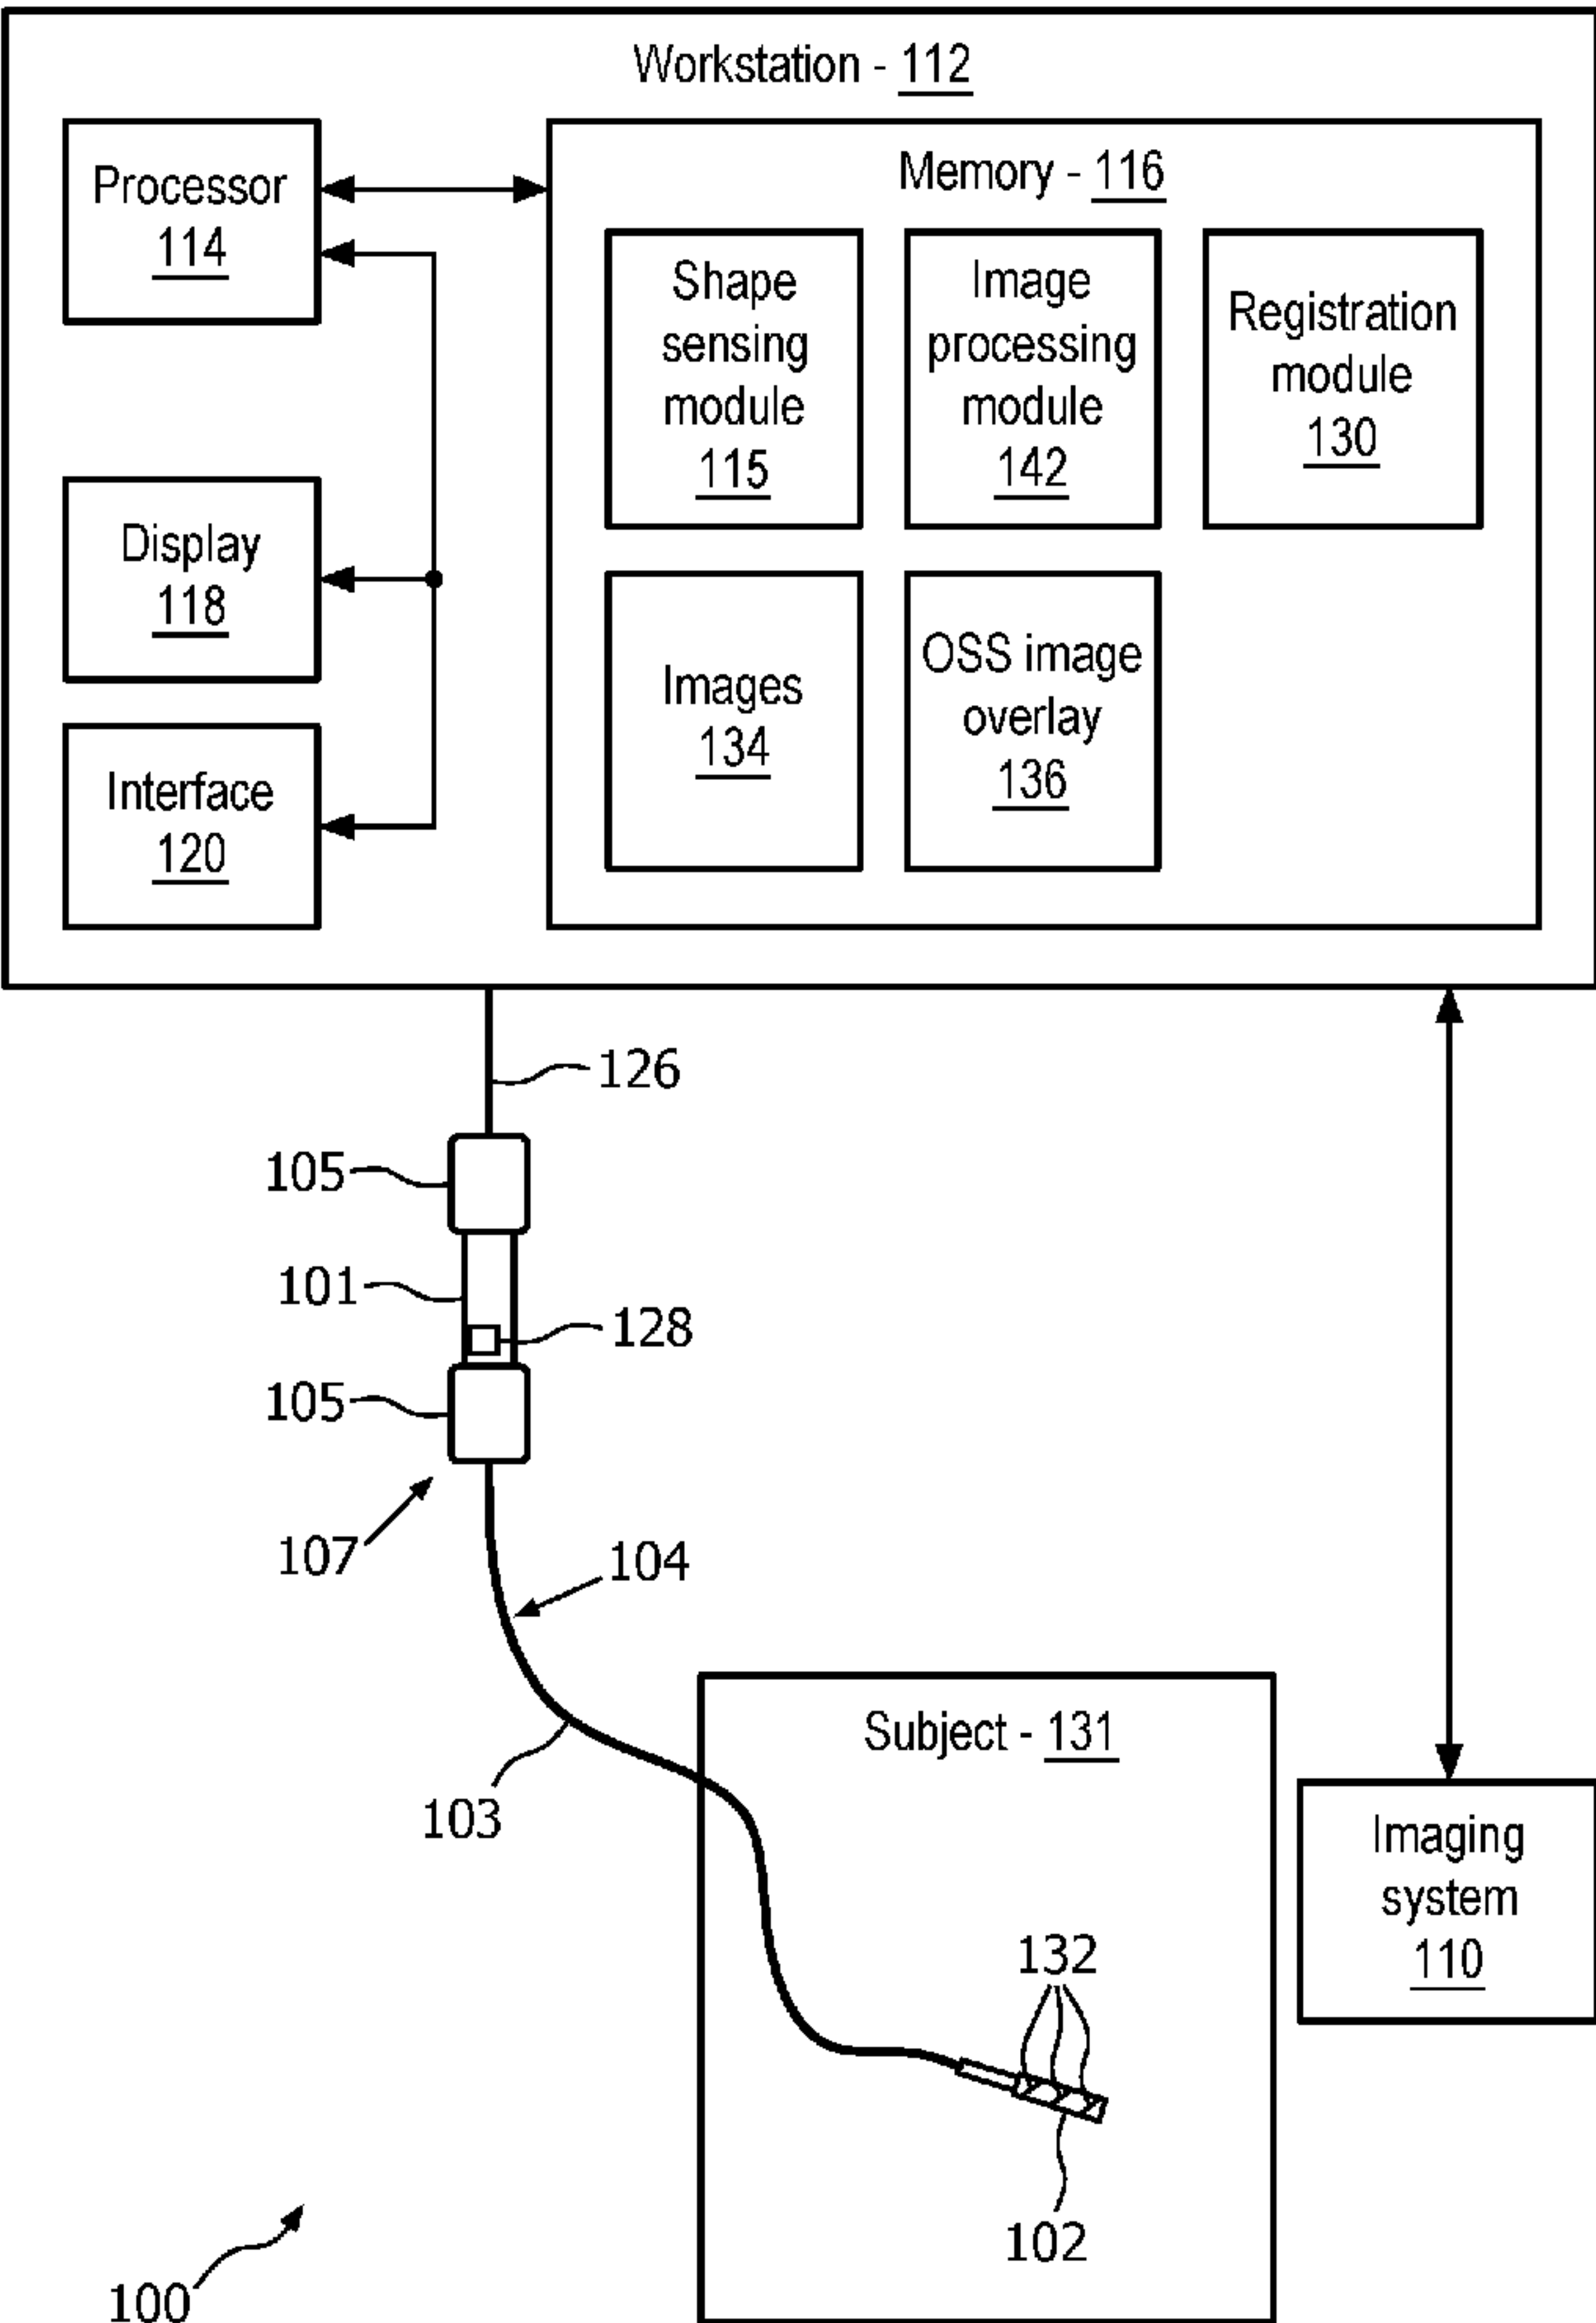

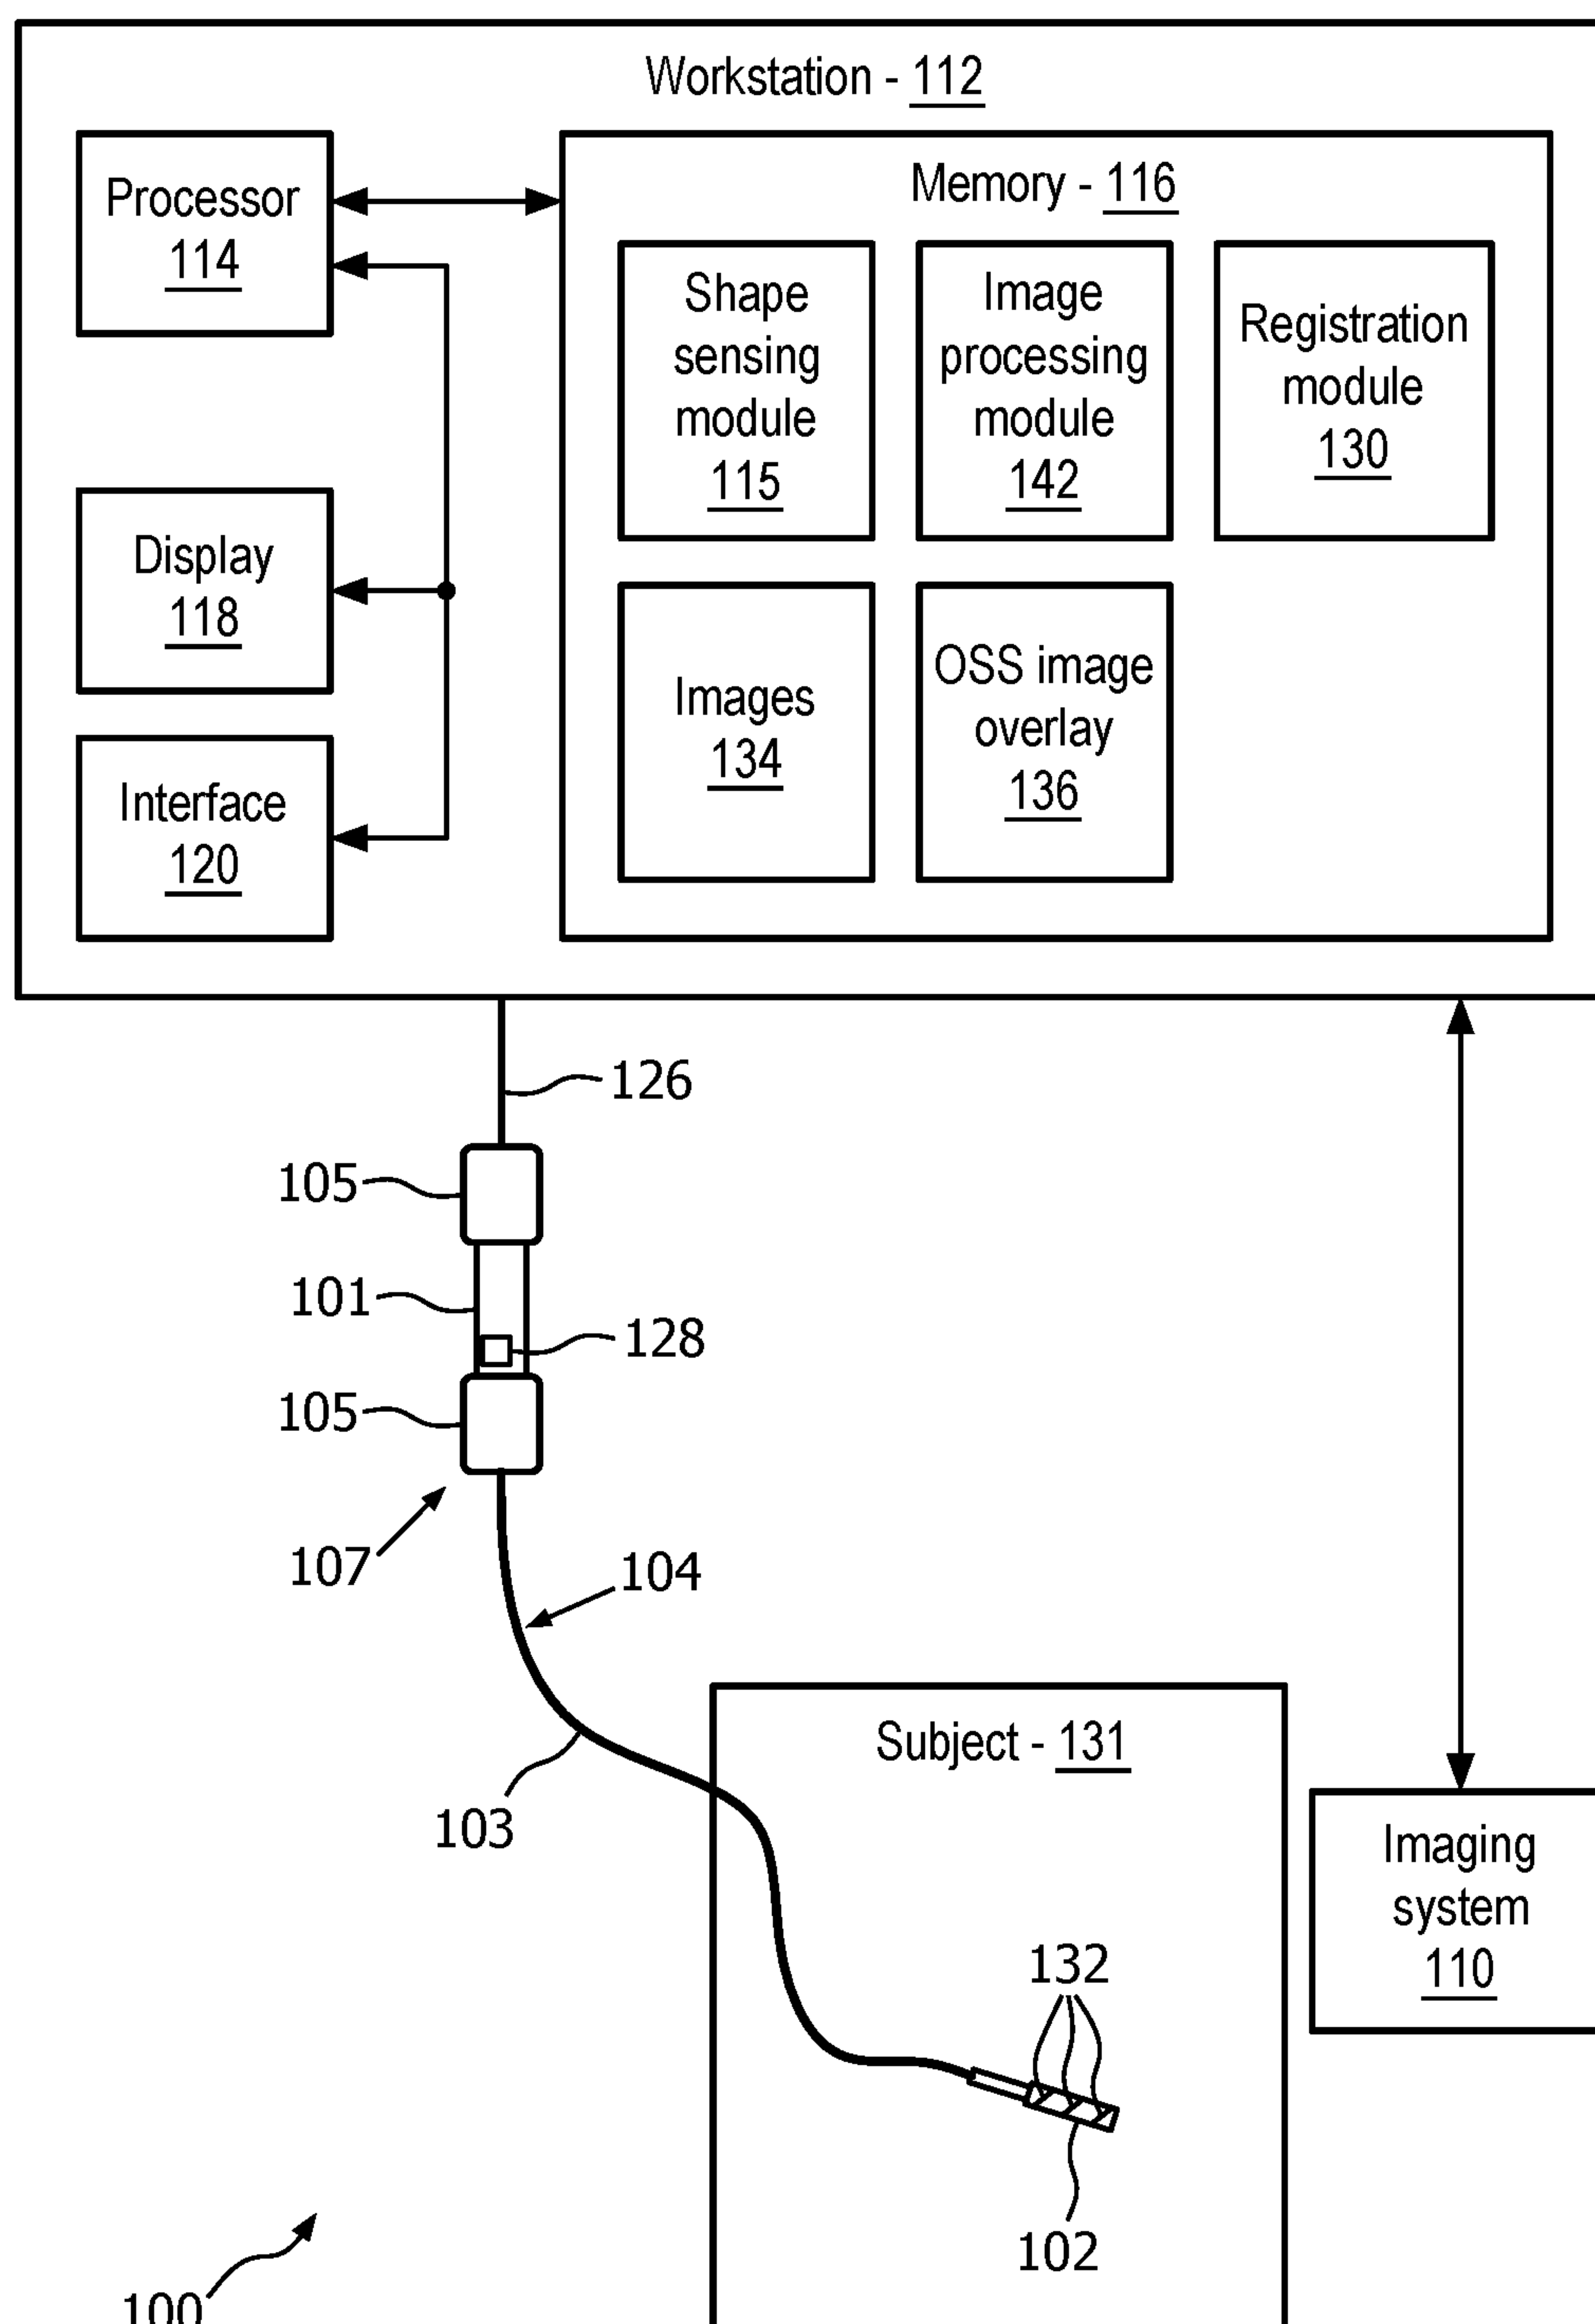


FIG. 1

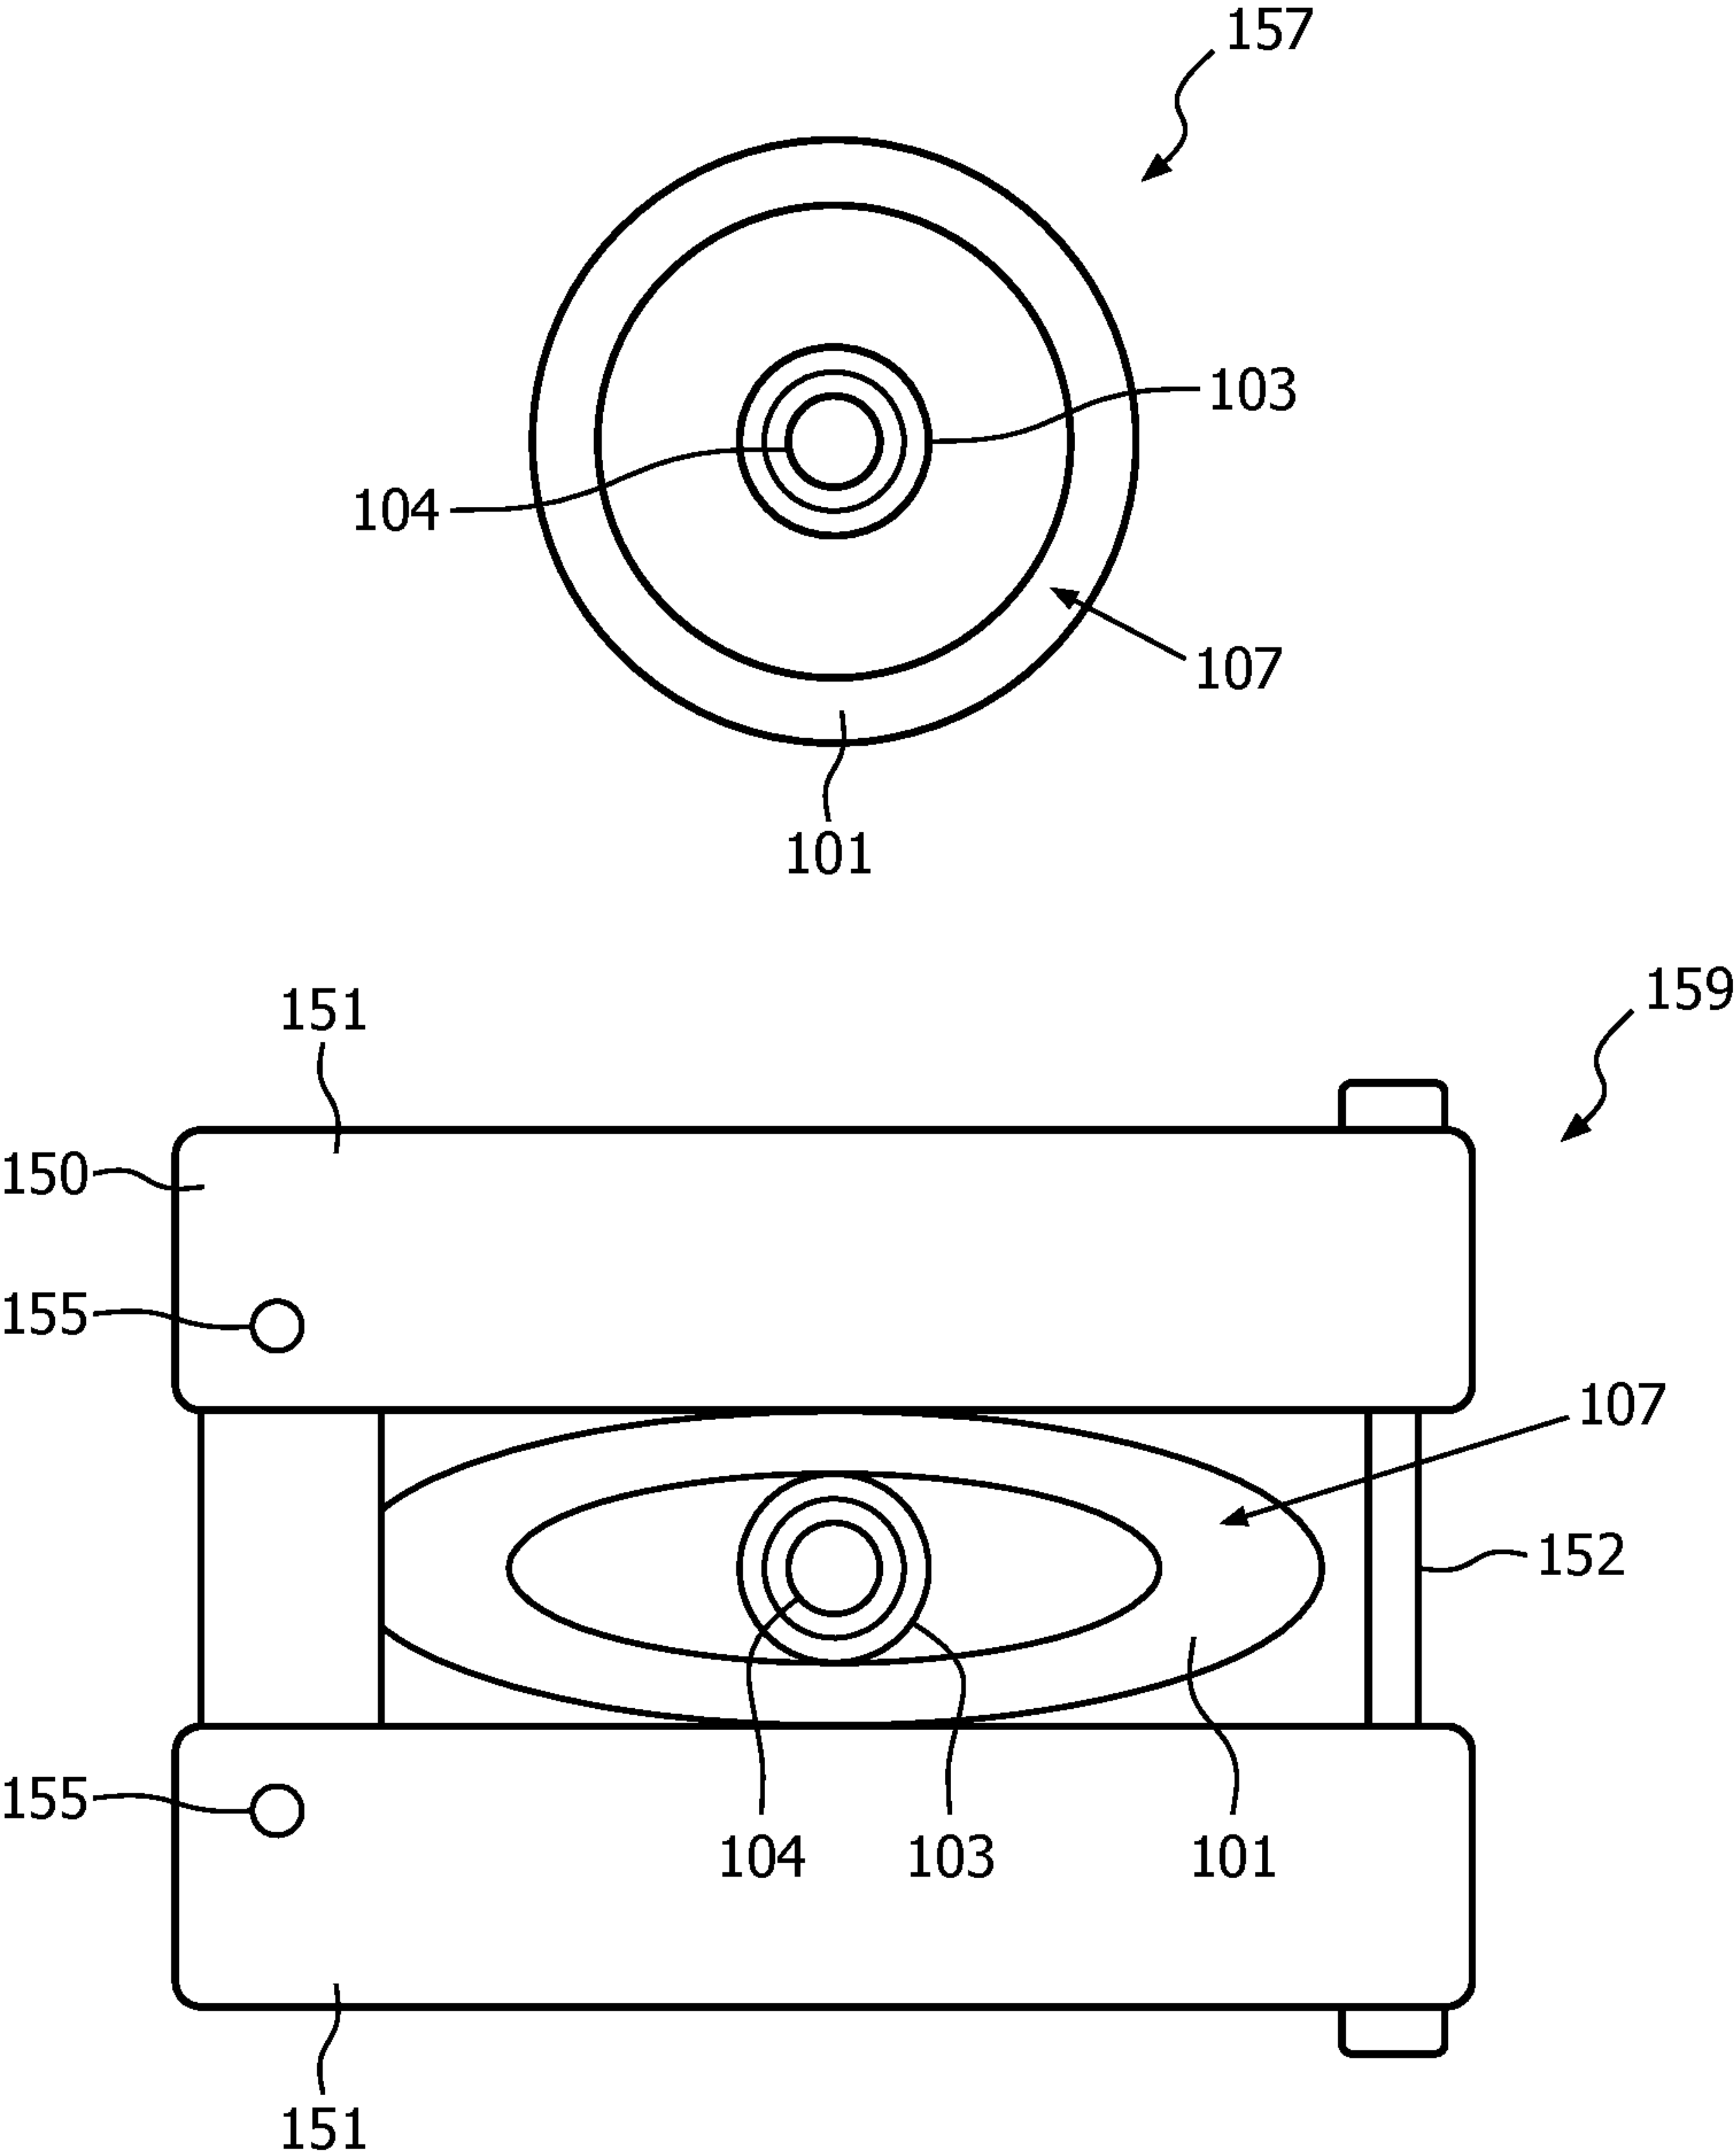


FIG. 2

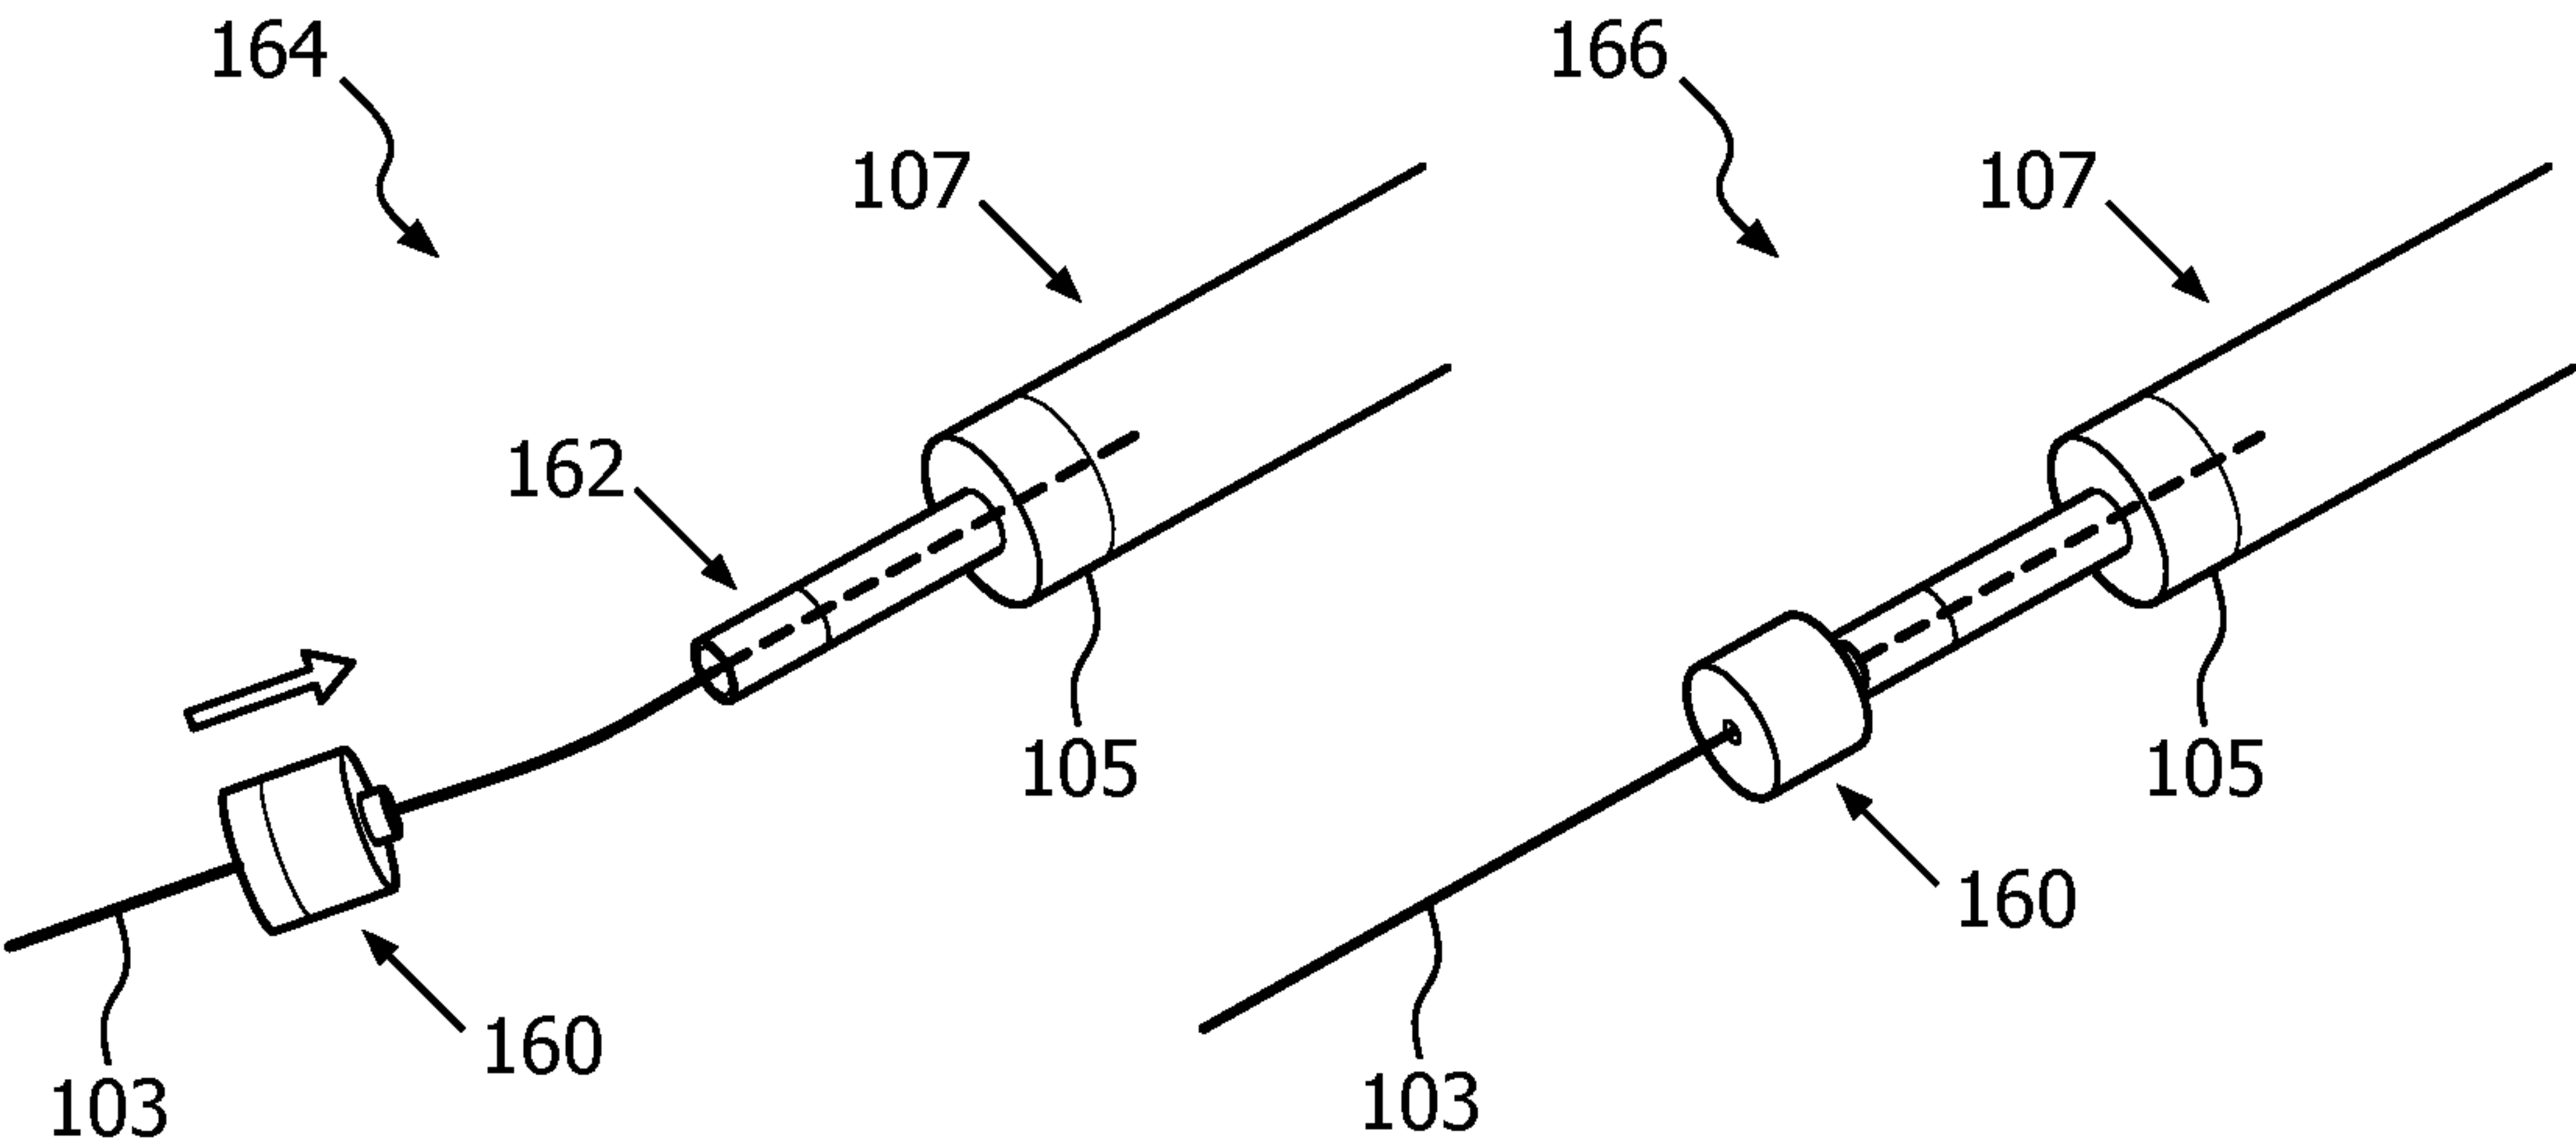


FIG. 3

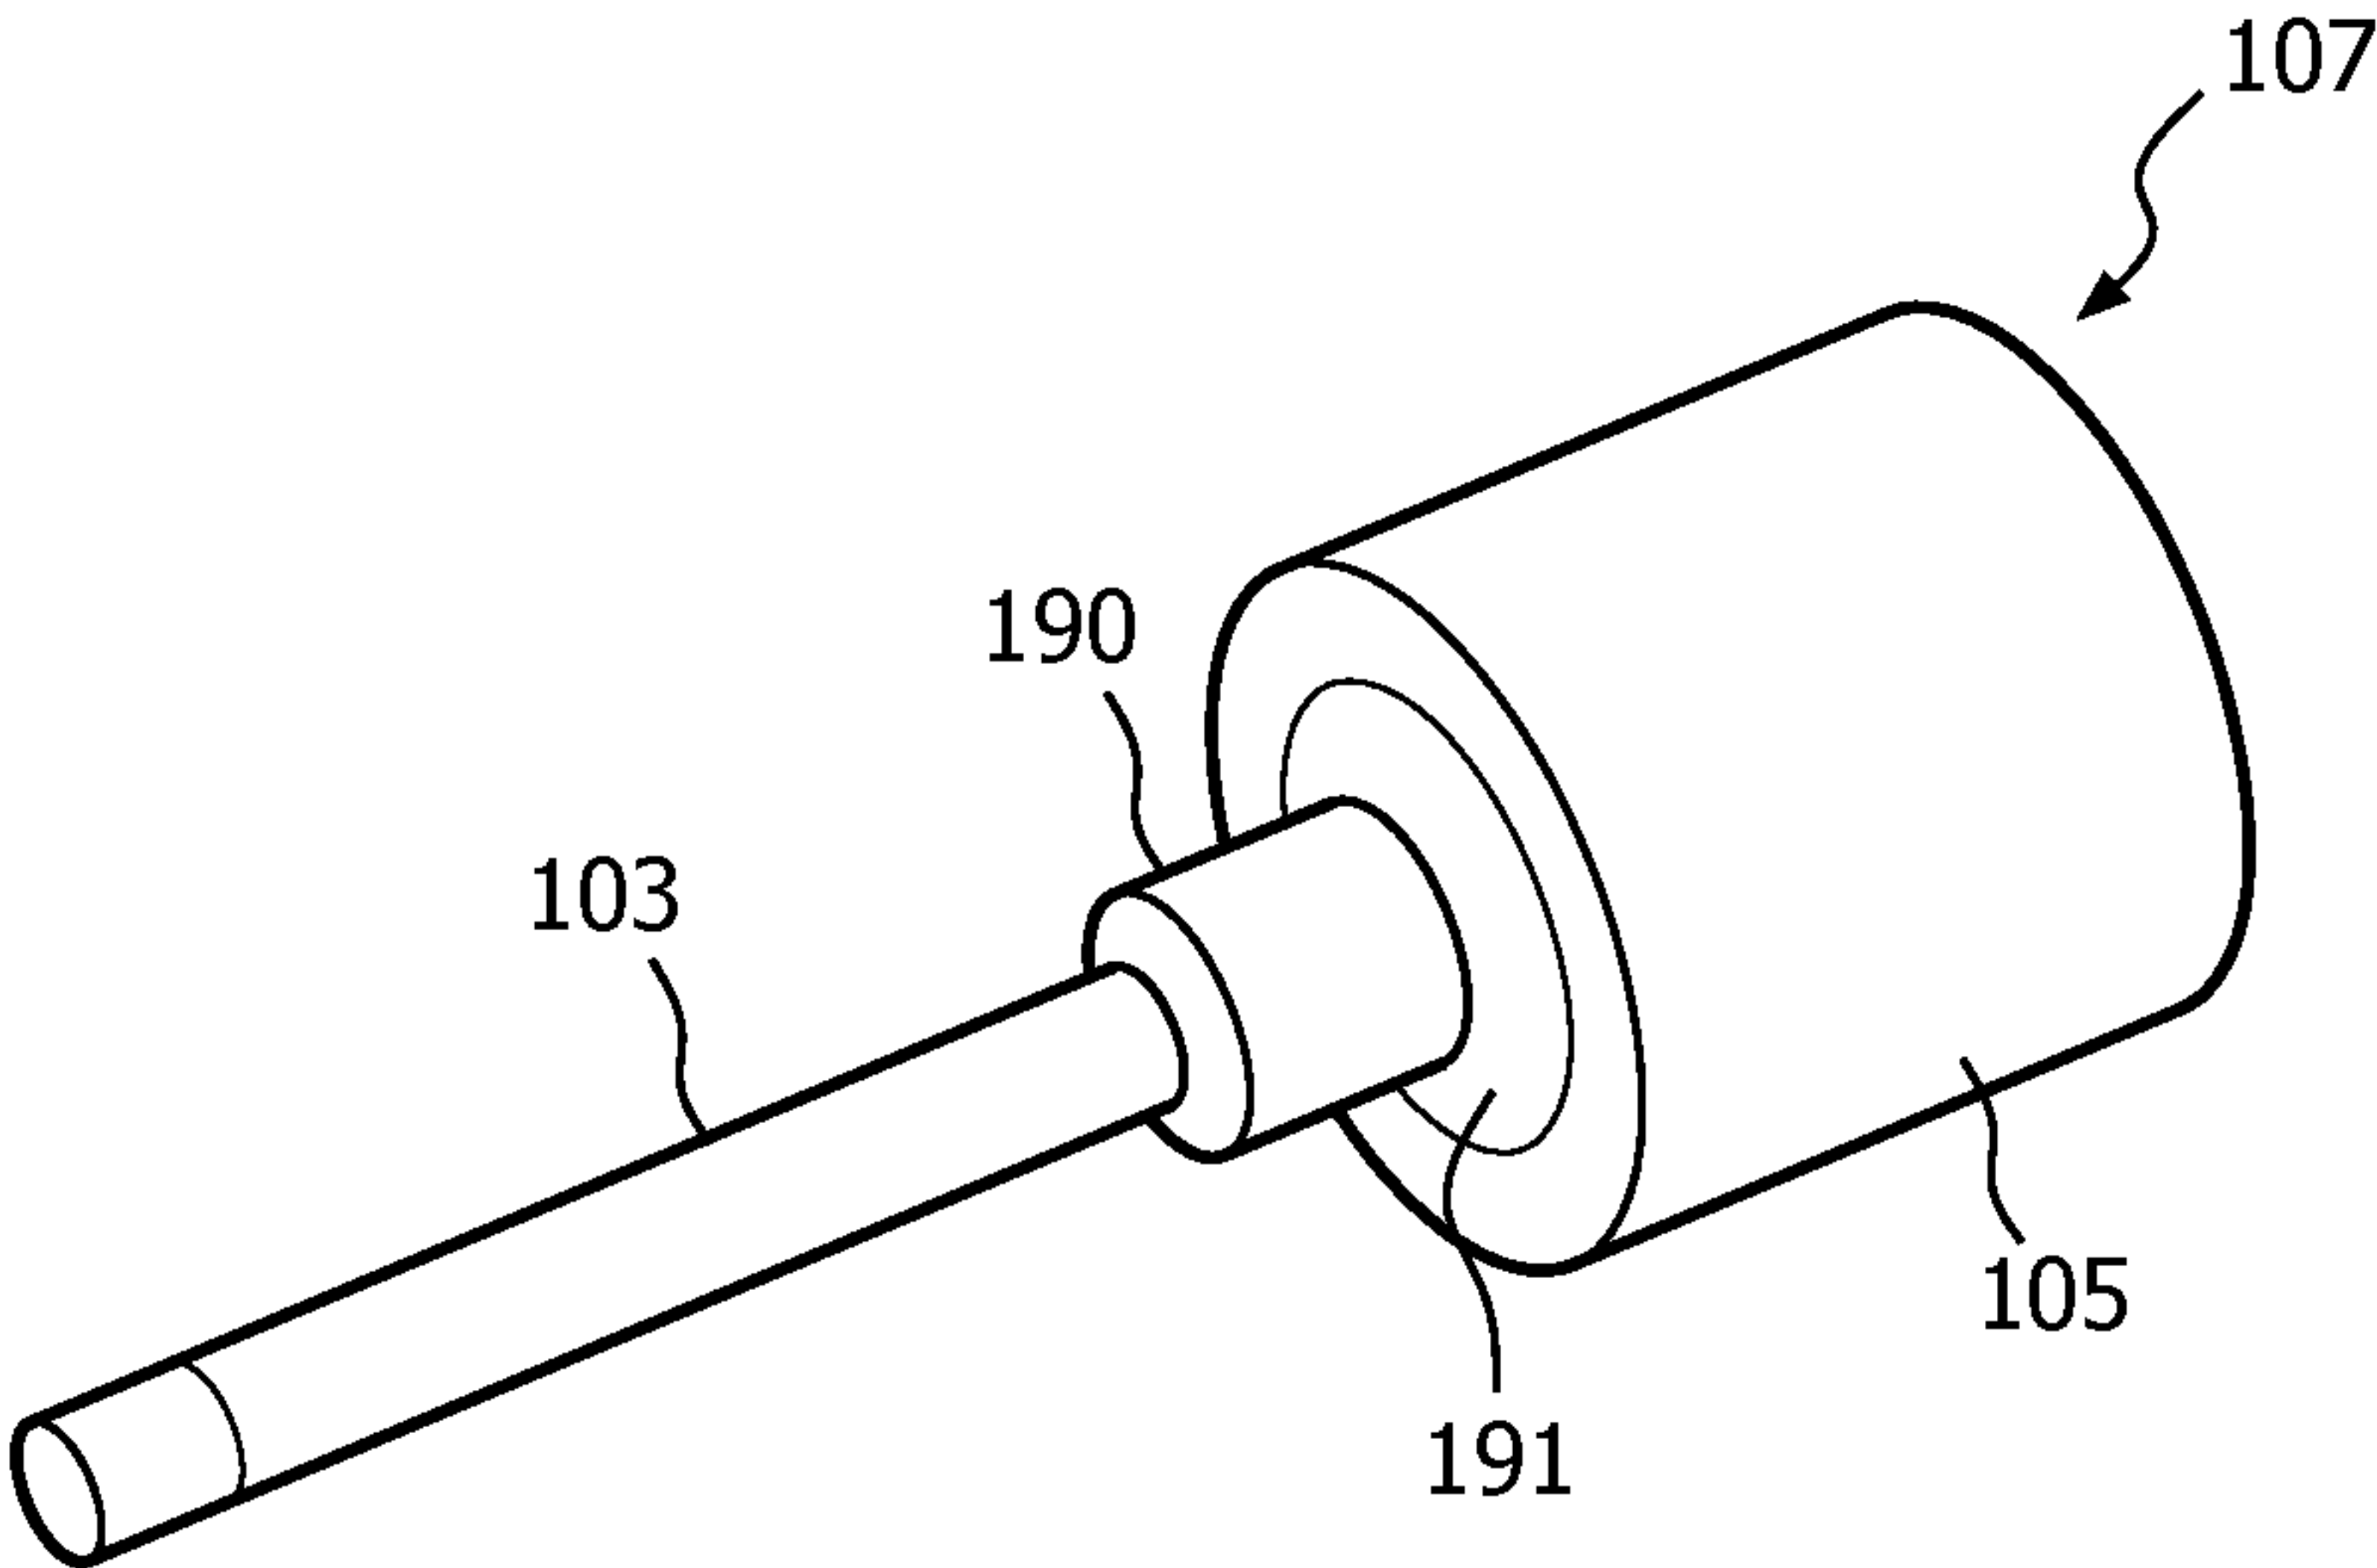


FIG. 4

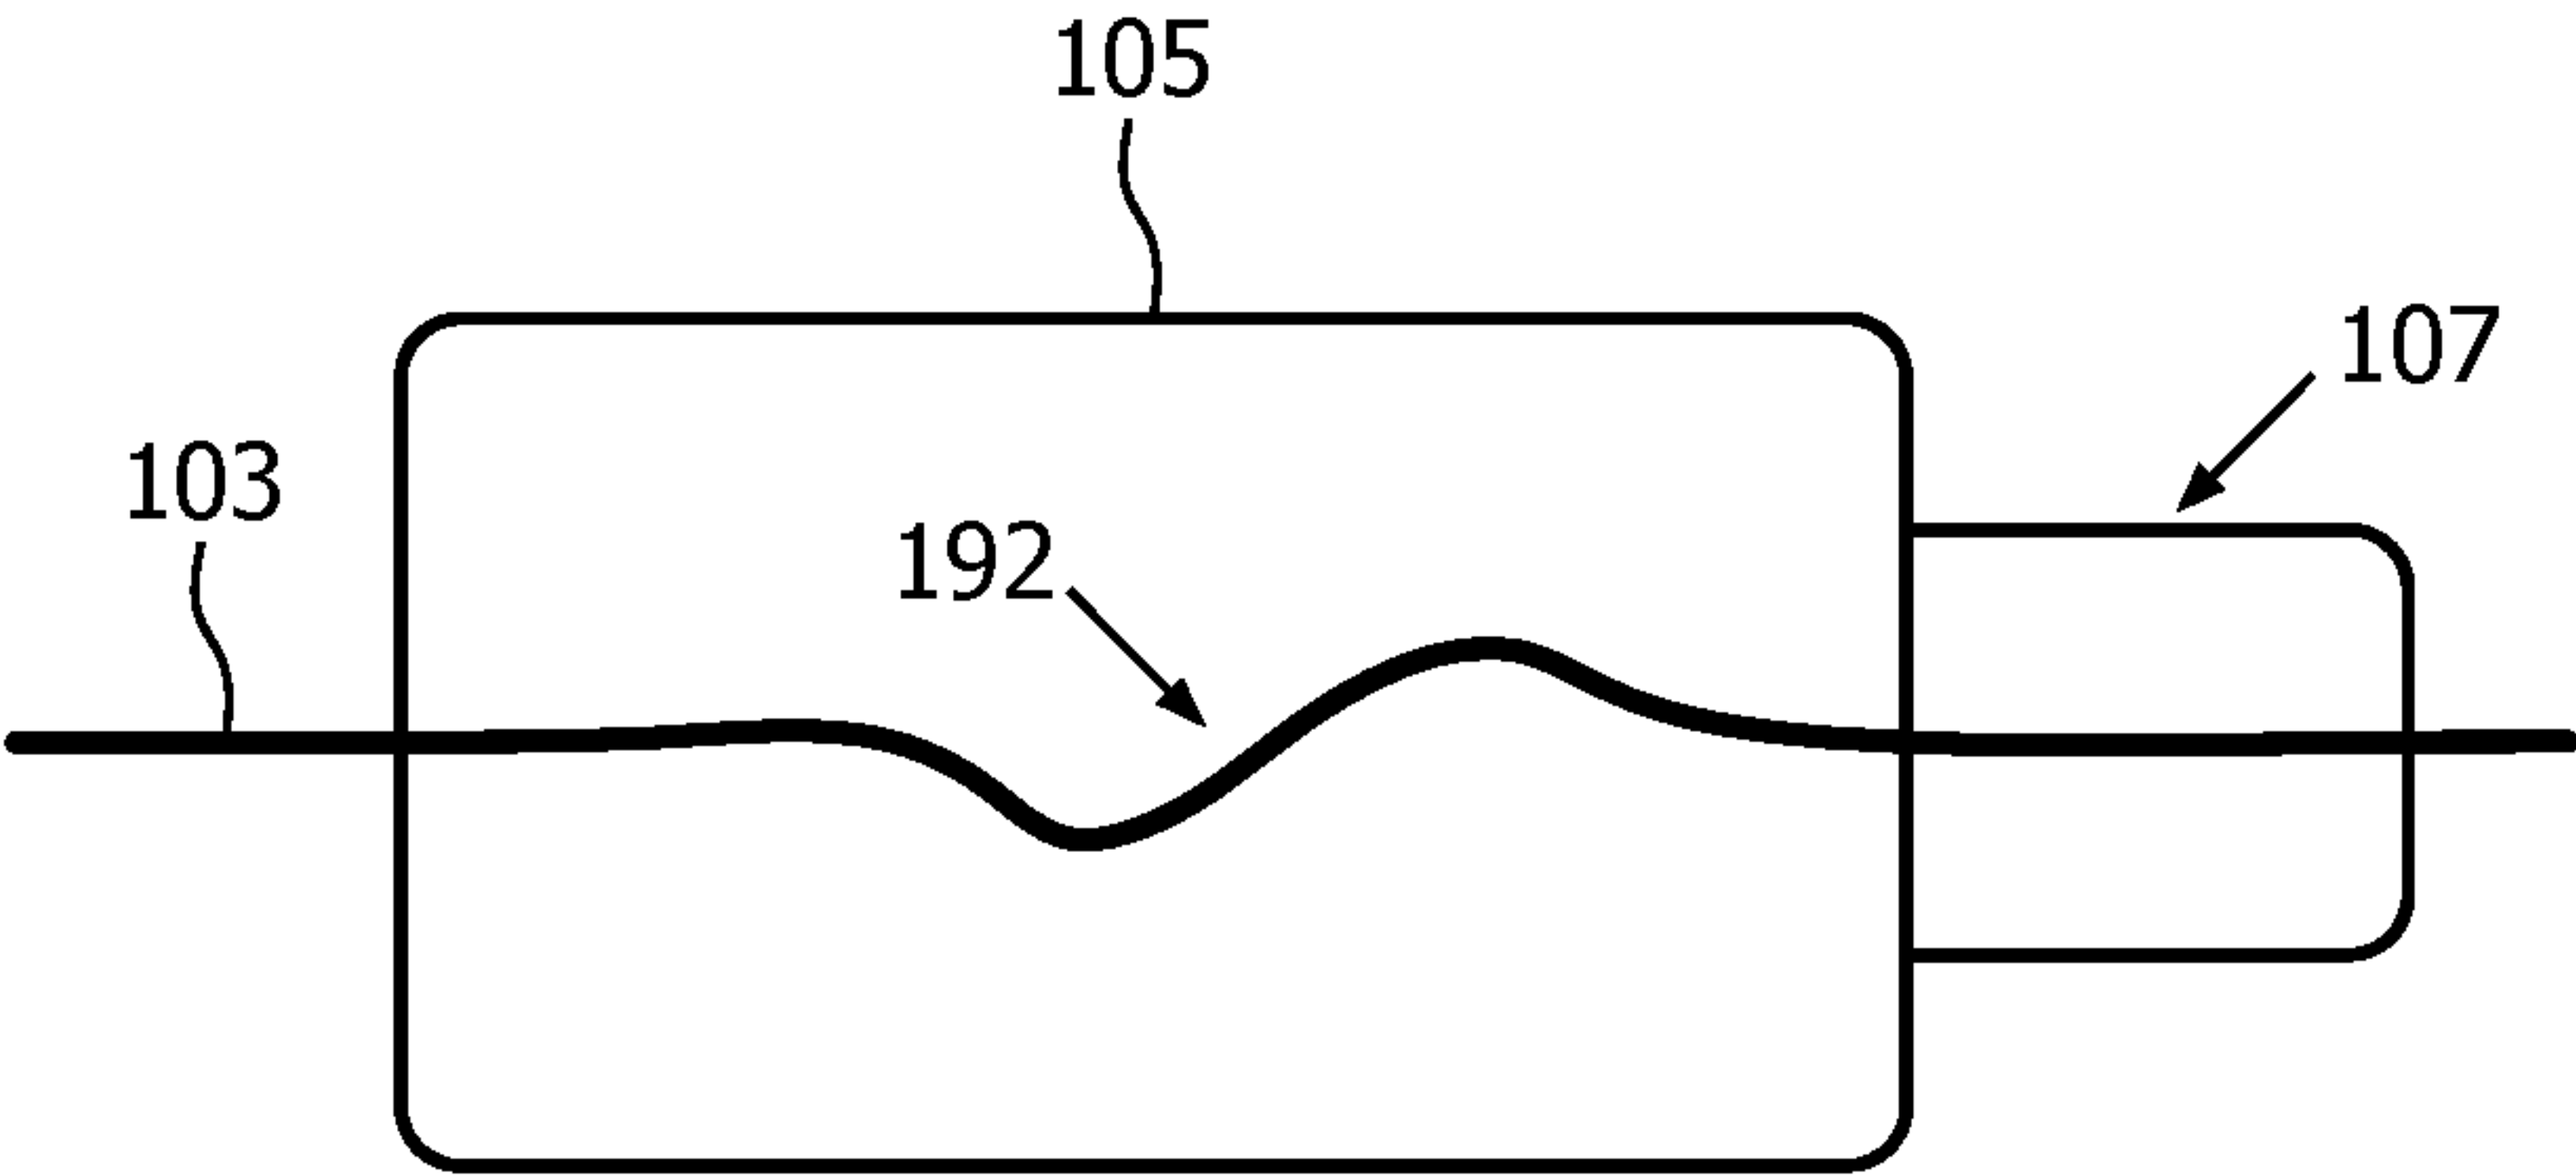


FIG. 5

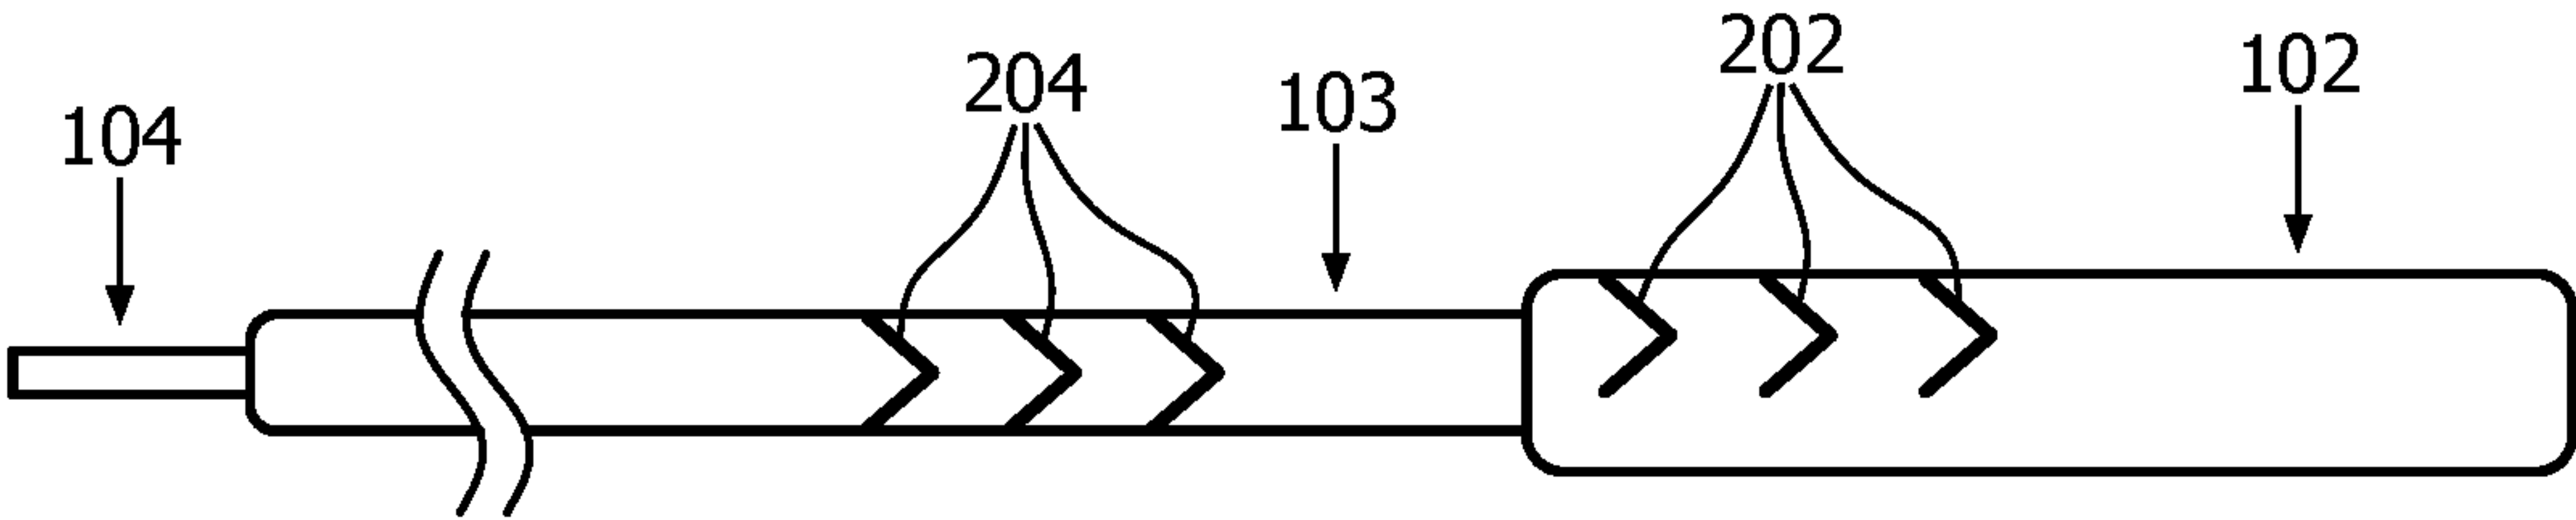


FIG. 6

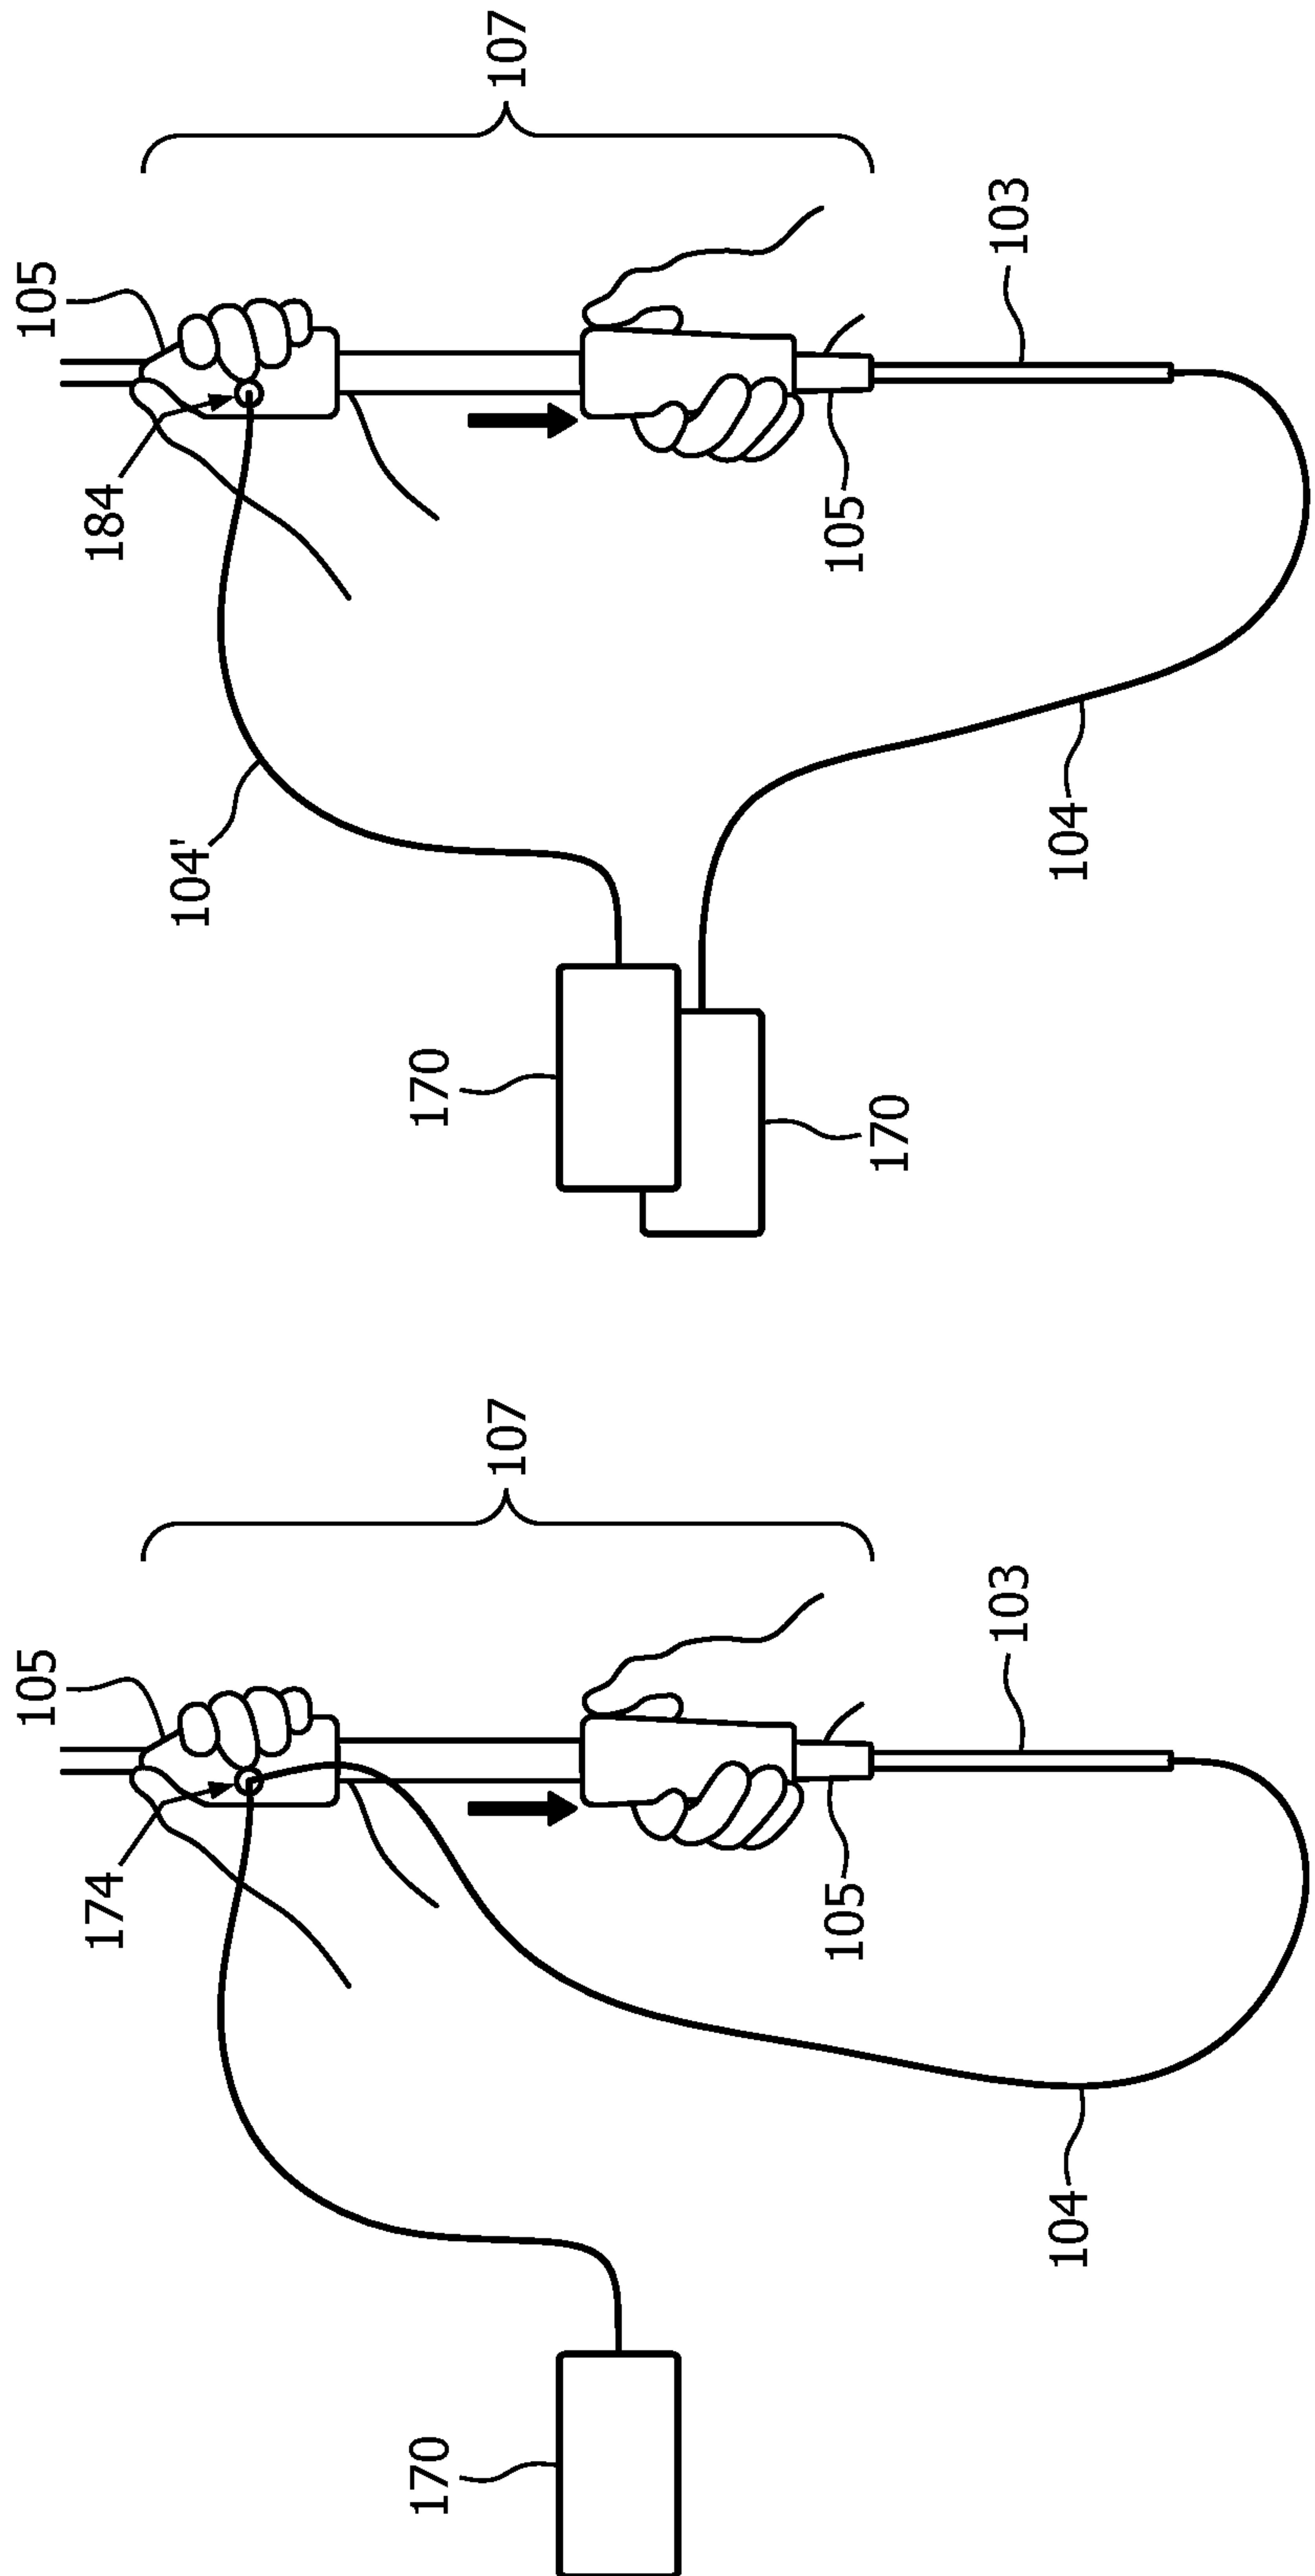
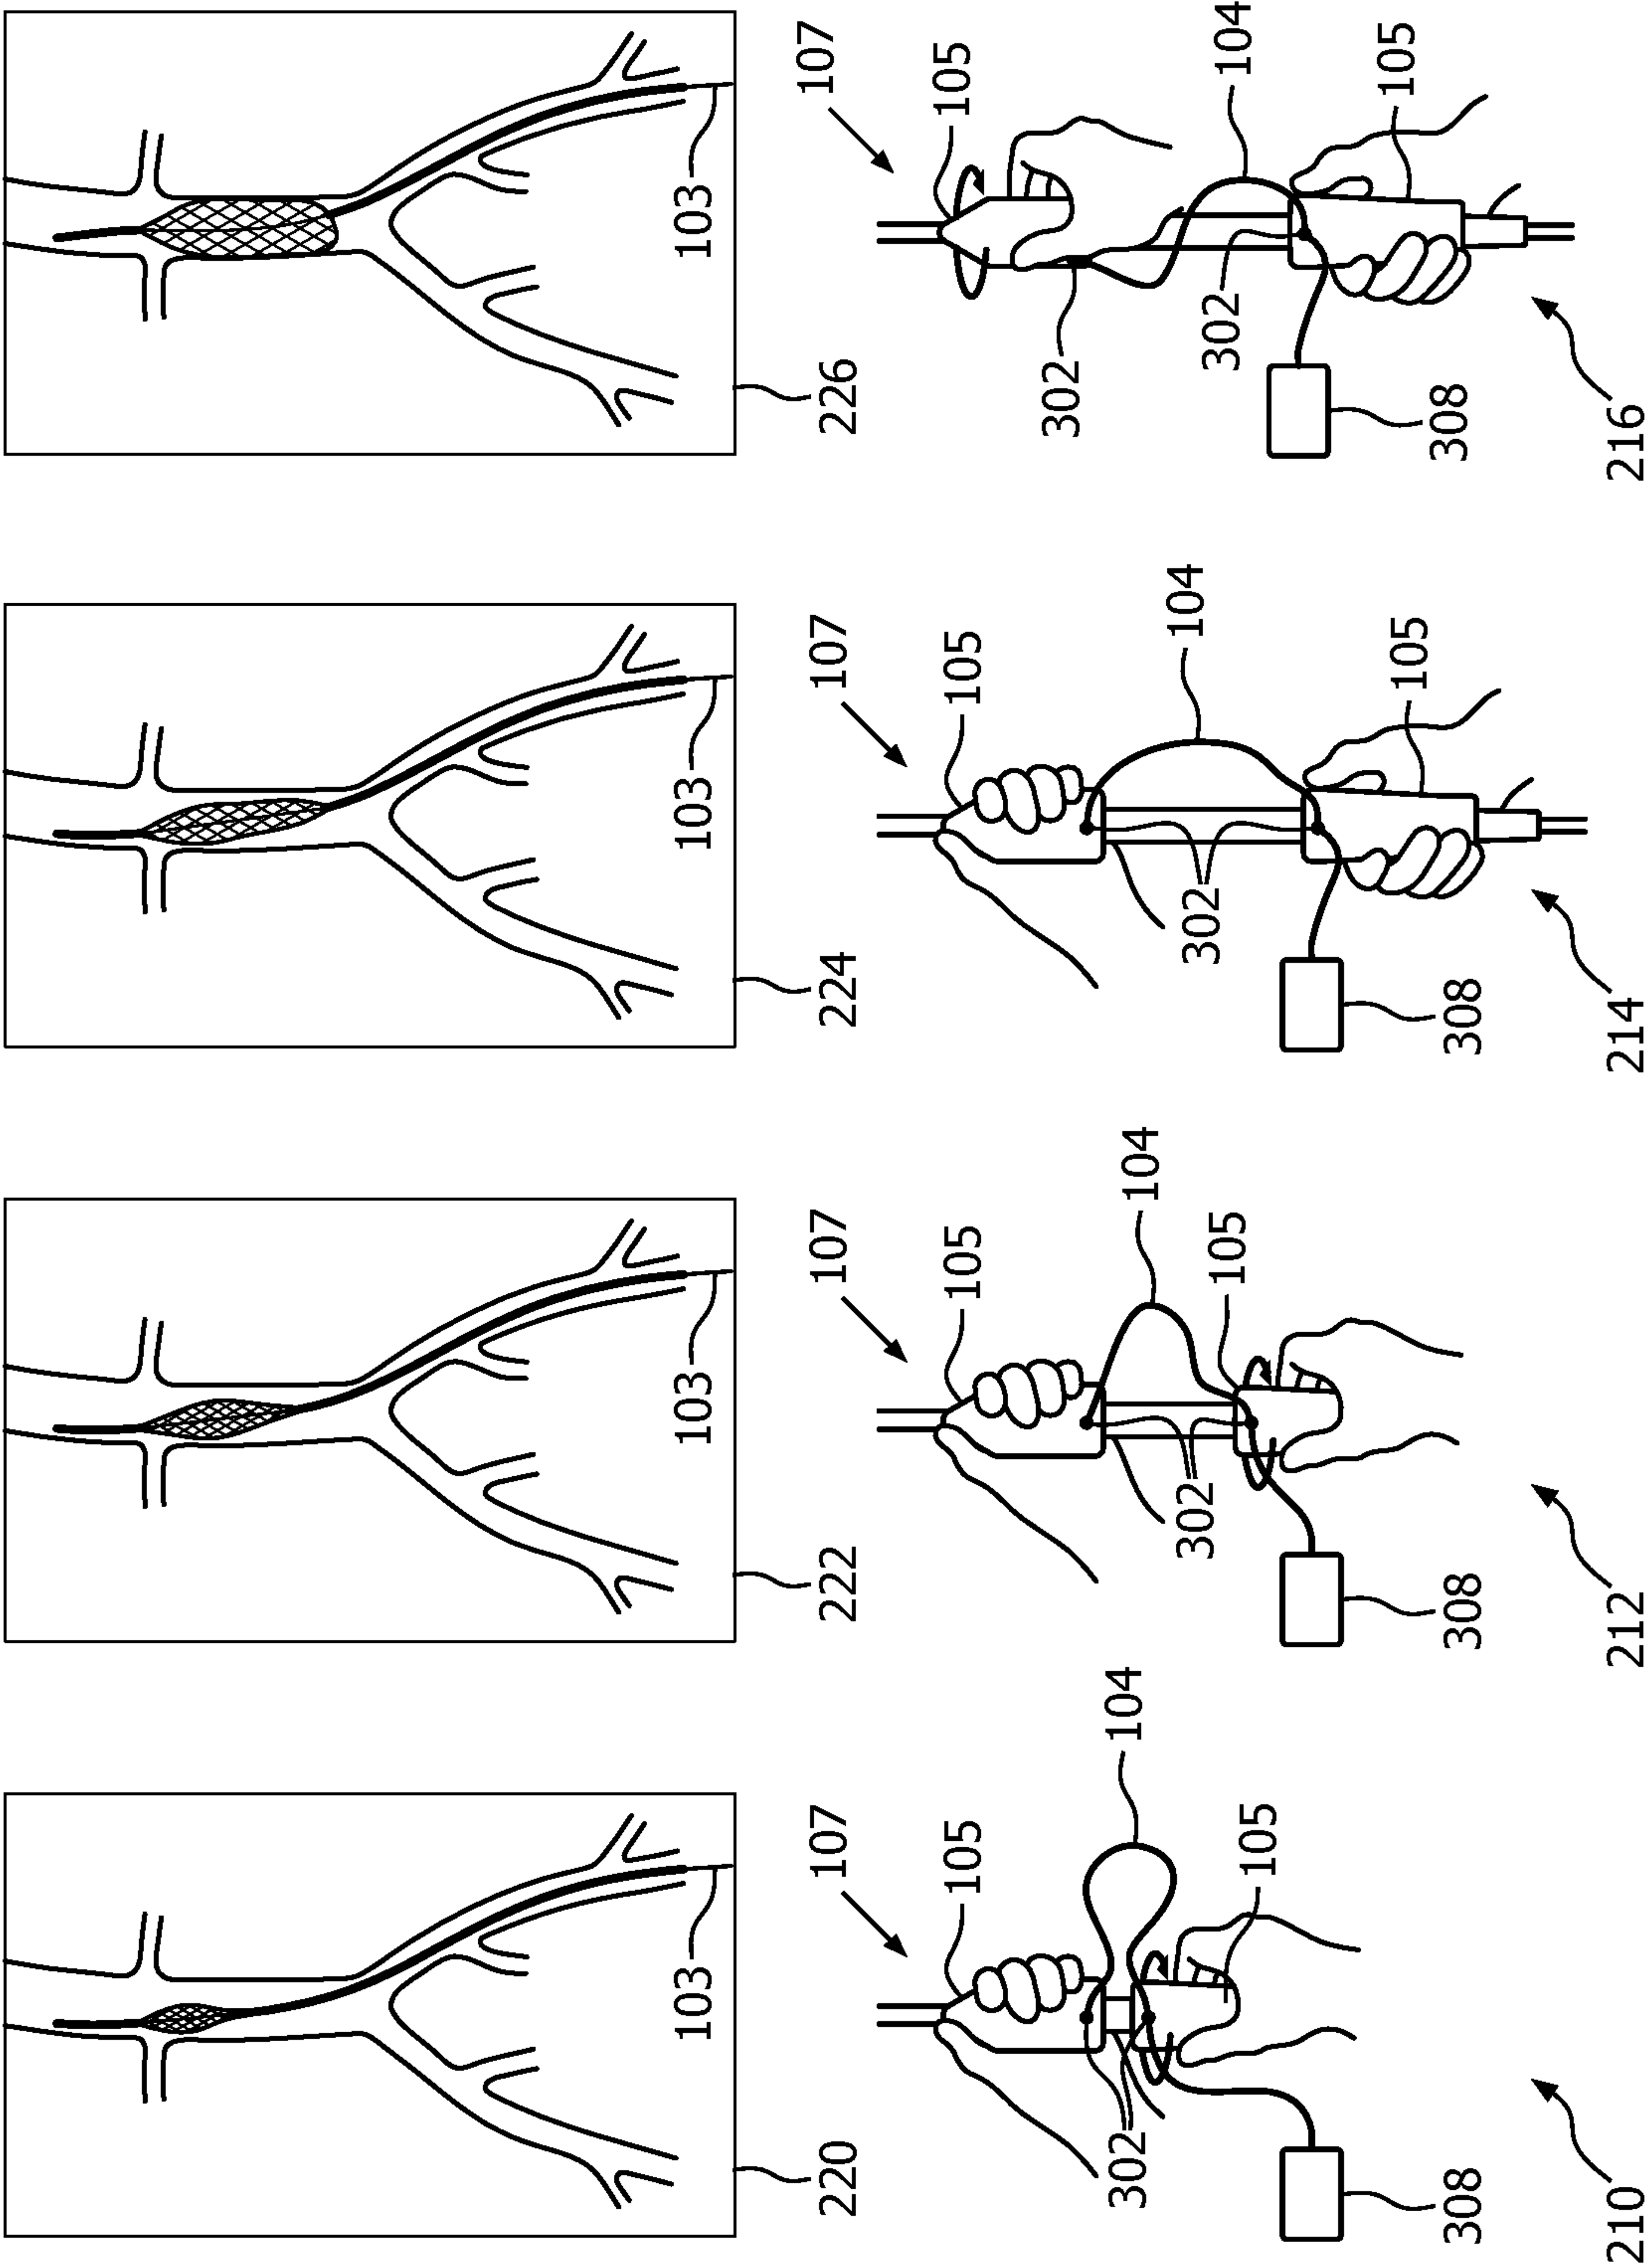


FIG. 8

FIG. 7



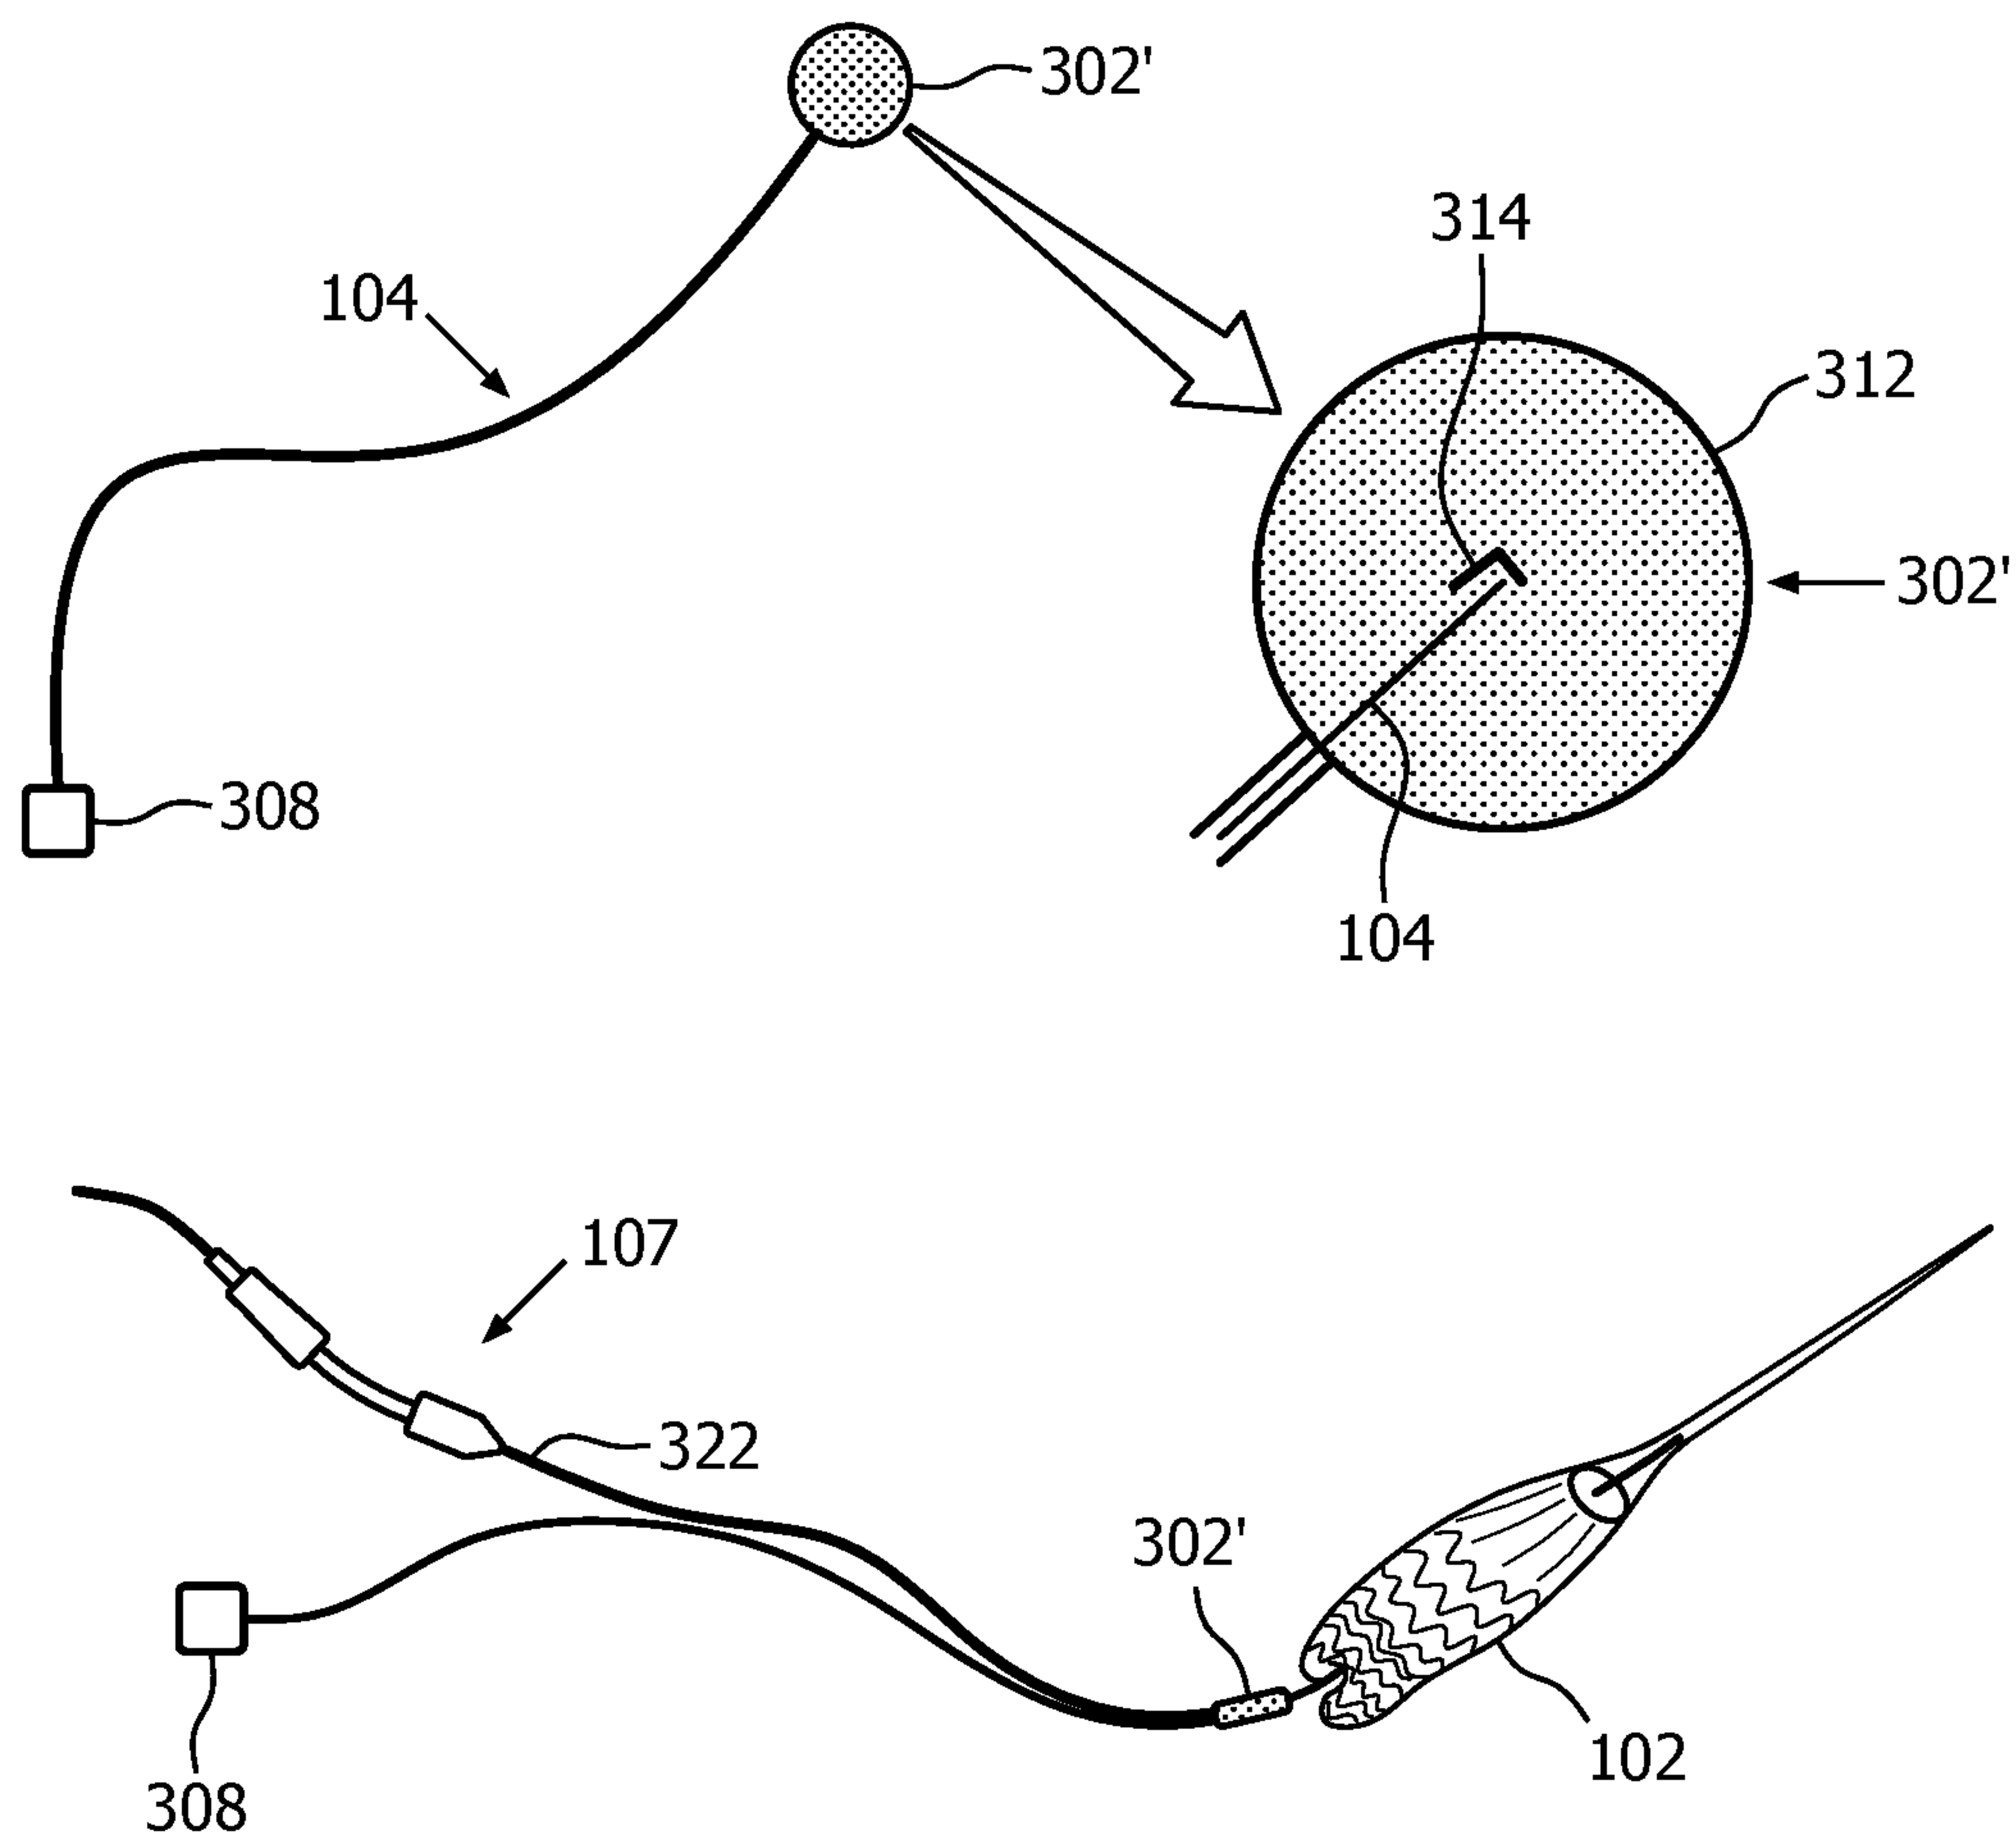


FIG. 10

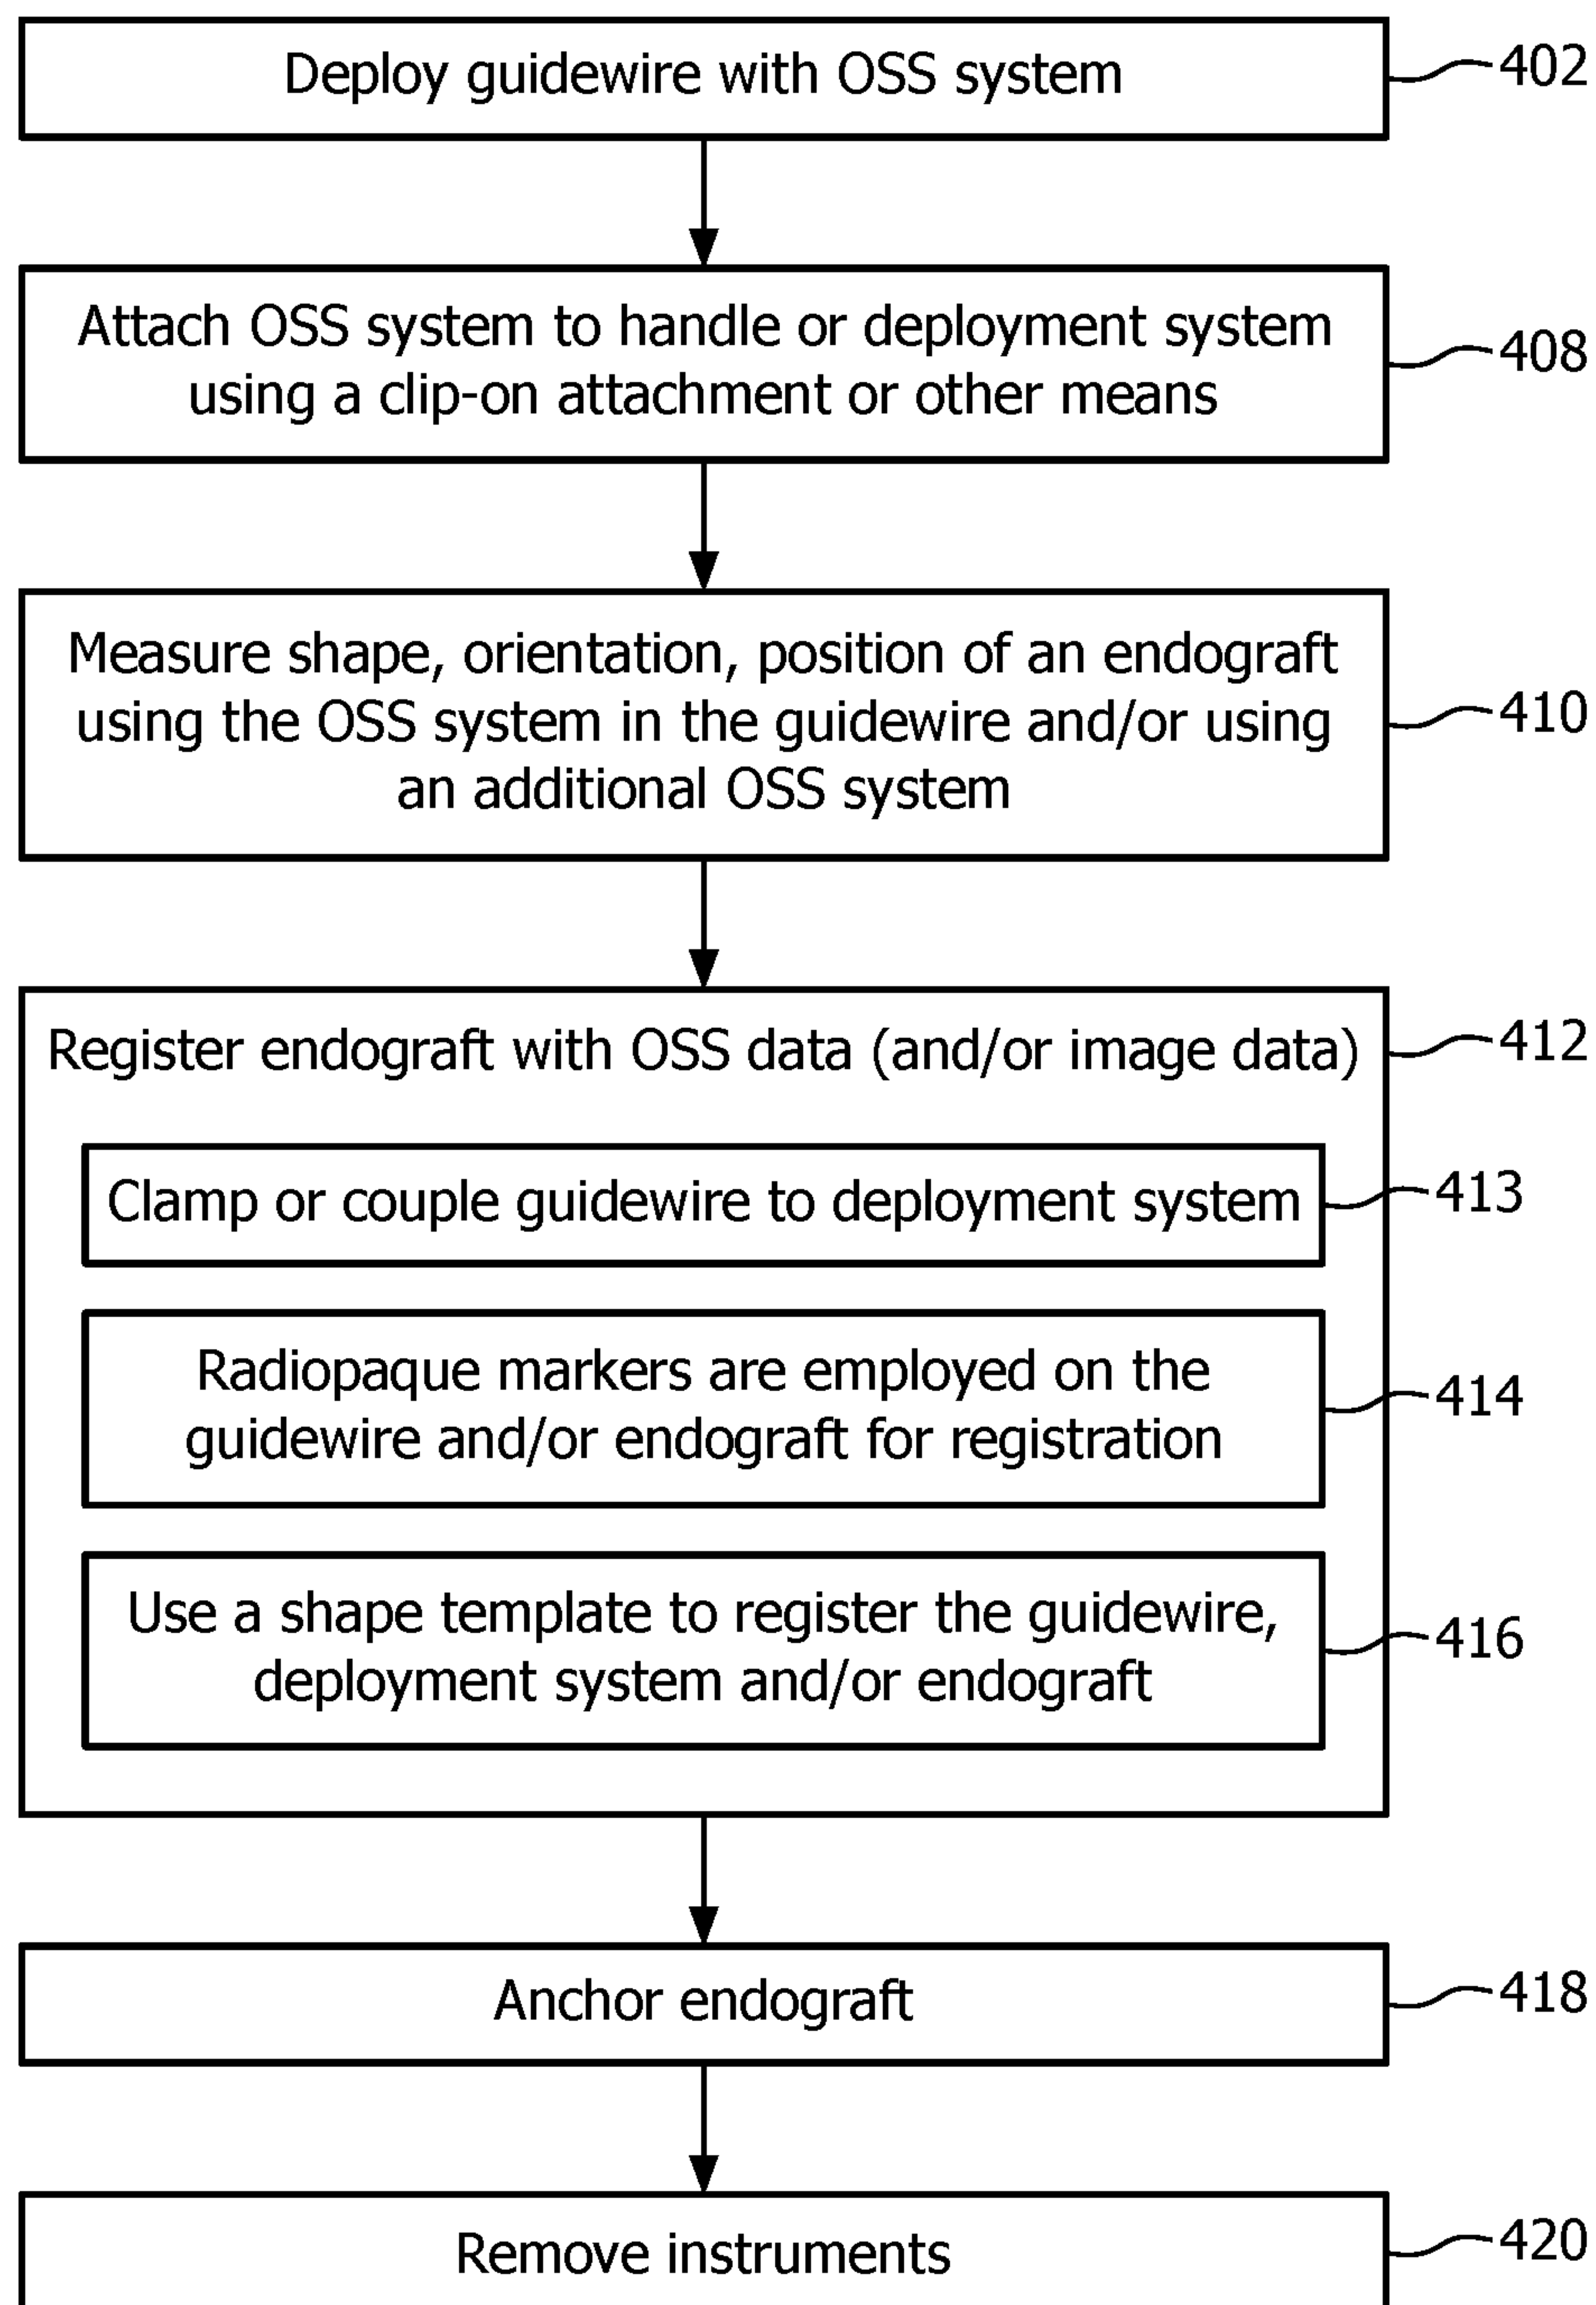


FIG. 11

DEVICE VISUALIZATION THROUGH OPTICAL SHAPE SENSING OF A GUIDEWIRE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation of and claims priority under 35 U.S.C. § 120 to U.S. application Ser. No. 15/544,925 filed on Jul. 20, 2017. U.S. patent application Ser. No. 15/544,925 is the U.S. National Phase application under 35 U.S.C. § 371 of International Application Serial No. PCT/IB2015/060063, filed on Dec. 31, 2015, which claims the benefit of priority under 35 U.S.C. § 119(e) to U.S. Application Ser. No. 62/106,267, filed on Jan. 22, 2015. The entire disclosures of U.S. application Ser. No. 15/544,925, U.S. Application Ser. No. 62/106,267 and International Application Serial No. PCT/IB2015/060063 are hereby specifically incorporated by reference herein.

BACKGROUND

Technical Field

[0002] This disclosure relates to medical instruments and more particularly to systems, devices and methods for medical device placement/deployment with shape sensing optical fibers integrated into a guidewire, in some instances with retrofit attachments onto the device.

Description of the Related Art

[0003] Optical shape sensing (OSS) uses light along a multicore optical fiber for device localization and navigation during surgical intervention. One principle involved makes use of distributed strain measurement in the optical fiber using characteristic Rayleigh backscatter or controlled grating patterns. The shape along the optical fiber begins at a specific point along the sensor, known as the launch point (or $z=0$), and the subsequent shape position and orientation are relative to that point. For meaningful clinical use, shape-sensed devices may be registered to an imaging frame of reference (such as a pre-operative CT or a live fluoroscopy image).

[0004] Endovascular aneurysm repair (EVAR) has replaced open surgery as the most common technique for the repair of abdominal aortic aneurysms (AAA). The procedure is typically carried out under x-ray fluoroscopy guidance and uses significant amounts of contrast to position and deploy the stent graft correctly. On average 50-100 mL of contrast dye is used during an EVAR procedure, which may result in acute renal failure in rare cases.

[0005] The most common complication from EVAR is endoleaks resulting from an insufficient seal of the stent graft to the aorta. Endoleaks involve incorrect flow around the stent (for example, flow around the stent at the proximal or distal attachment site, flow through the graft wall, retrograde flow from the branches, etc.).

[0006] Another complication around EVAR involves ischemia of the aortic side branches (such as the colonic, renal, and pelvic arteries). This can occur due to misplacement of the stent graft such that the stent partially or completely covers one of the side vessels. This is associated with a lack of high-quality imaging technology as well as the experience of the endovascular team.

[0007] In EVAR, endografts are contained within a deployment system that is used to navigate the endograft to the correct part of the vasculature. The deployment systems tend to be relatively large and stiff endovascular devices. They typically involve a handle or set of knobs and dials at the proximal end to control the various steps around the deployment. The endograft lies within a distal part of the device and is only released once the device has been navigated to the appropriate location. In some cases, the endograft completely deploys in one step, while in other cases the endograft can be partially deployed to allow for correct positioning and orientation before the final deployment step firmly attaches the endograft to the vasculature (typically through a retaining/sealing ring).

[0008] The endograft typically requires a sufficient amount of healthy vasculature where it can land its sealing ring. If this is not possible beneath the renal arteries, then the stent will cover those arteries, and must create some alternative way of maintaining flow to those vessels. This can be done with a fenestrated endograft (e.g., a endograft with windows for the side-branches) in a procedure known as fenestrated endovascular aneurysm repair (FEVAR). In this case, the endograft has fenestrations that must be lined up correctly with the side branches and additional stents are placed to connect the side vessels to the main stent.

[0009] Under x-ray guidance the endograft can be visualized through x-ray visible markers that are located in key positions on the stent. In a fenestrated stent, the markers identify the locations of the fenestrations and can be used to orient the endograft to appropriately align the fenestrations with the side vessels. Complications from EVAR includes misplacement of the endograft resulting in endoleaks, misplacement of the endograft resulting in occlusion of the side branches, contrast nephropathy due to high levels of contrast used during endograft deployment and high contrast and radiation dose due to long procedure times due to navigation and deployment in a complex anatomy. In addition, placement of a three-dimensional endograft within a three-dimensional anatomy is challenging and is typically performed under two-dimensional imaging guidance through x-ray fluoroscopy.

SUMMARY

[0010] In accordance with the present principles, a medical device deployment system includes a main body and a guidewire capable of being passed through the main body and including a lumen. An optical shape sensing (OSS) system is configured to pass through the lumen in the guidewire. The OSS system is configured to measure at least one of shape, position or orientation of an endograft relative to a blood vessel for placement of the endograft.

[0011] An endograft deployment system includes a workstation including a processor and memory. An optical shape sensing module is stored in memory and configured to interpret optical shape sensing data. A deployment system includes a tube. A guidewire is capable of being passed through the tube, and the guidewire includes a lumen. An optical shape sensing (OSS) system is configured to pass through the lumen in the guidewire. The OSS system is configured to measure at least one of shape, position or orientation of an endograft relative to a blood vessel for placement of the endograft. A registration module is configured to register the optical shape sensing data to pre-operative or intra-operative images.

[0012] A medical device deployment system includes a main body having a control handle coupled to the main body. An optical shape sensing (OSS) system is configured to measure at least one of shape, position or orientation of an endograft relative to a blood vessel for placement of the endograft. At least one clip-on attachment is configured to attach the OSS system to the control handle.

[0013] A method for endograft deployment includes deploying a guide wire having an optical shape sensing (OSS) system within a lumen of the guide wire, the guide wire configured to deliver an endograft into a vessel; measuring at least one of shape, position or orientation of the guide wire using the OSS system to identify a shape, position or orientation of the endograft during deployment; registering OSS data with image data on the vessel where the endograft is placed; anchoring the endograft in the blood vessel; and removing the guidewire and the OSS system from the vessel.

[0014] These and other objects, features and advantages of the present disclosure will become apparent from the following detailed description of illustrative embodiments thereof, which is to be read in connection with the accompanying drawings.

BRIEF DESCRIPTION OF DRAWINGS

[0015] This disclosure will present in detail the following description of preferred embodiments with reference to the following figures wherein:

[0016] FIG. 1 is a block/flow diagram showing a system configured for endograft placement/deployment using an optical shape sensing system within a guidewire in accordance with one embodiment;

[0017] FIG. 2 is a diagram showing a cross-section of an unclamped and a clamped assembly having an OSS system, guidewire and tube of a deployment system in accordance with one embodiment;

[0018] FIG. 3 is a diagram showing a guidewire coupling mechanism prior to and after engagement with a deployment system in accordance with one embodiment;

[0019] FIG. 4 is a perspective view showing a rotational sensor assembly between a guidewire and a handle of a deployment system in accordance with one embodiment;

[0020] FIG. 5 is a side cross-sectional view showing a shape template for a guidewire within a handle of a deployment system in accordance with one embodiment;

[0021] FIG. 6 is a side view showing a guidewire and an endograft with radiopaque registration markers in accordance with one embodiment;

[0022] FIG. 7 is a diagram showing an OSS system for a guidewire coupled to a handle of a deployment system in accordance with one embodiment;

[0023] FIG. 8 is a diagram showing an OSS system for a guidewire and an additional OSS system coupled to a handle of a deployment system in accordance with another embodiment;

[0024] FIG. 9 is a diagram showing relative positions of handles of a deployment system measured by an OSS system and corresponding model displays showing the relative effects in accordance with one embodiment;

[0025] FIG. 10 is a perspective view showing a clip-on attachment mechanism coupled to a deployment system and a magnified view of an OSS system with the clip-on attachment mechanism in accordance with one embodiment; and

[0026] FIG. 11 is a flow diagram showing a method for endograft placement/deployment using an optical shape sensing system in a guidewire in accordance with illustrative embodiments.

DETAILED DESCRIPTION OF EMBODIMENTS

[0027] In accordance with the present principles, a three-dimensional visualization of a stent (endograft) with respect to anatomic imaging (e.g., a pre-operative computed tomography (CT) image, an intra-operative xperCT/3DRA, a fluoroscopy roadmap, etc.) can be more accurately controlled during deployment using optical shape sensing (OSS). Introducing OSS for navigation to endovascular aneurysm repair (EVAR) can reduce radiation dose and provide a more intuitive way to position catheters and guidewires within a three-dimensional vasculature to reduce procedure times and improve outcomes.

[0028] One feature of EVAR procedures is the deployment of an endograft. The orientation and position of the endograft is an important consideration in making a good seal with the vessel and adjusting the flow such that an aneurysm is no longer under pressure. If the endograft is not positioned correctly, blood may leak around the endograft and continue to pool in an aneurysm sac, or the endograft could occlude side-vessels off the aorta which can cause poor blood flow to critical organs. In fenestrated endovascular aneurysm repair (FEVAR), side-branches (such as the renal arteries) need to be cannulated. This cannulation involves navigating a catheter and guidewire through a semi-deployed stent graft, exiting the endograft via a fenestration, and then entering the target vessel. While this can be done largely through the known position and shape of the devices through OSS, it may also be advantageous to see the position of the endograft (and corresponding fenestrations). Thus, by shape sensing the endograft, the endograft position/orientation/shape can be tracked during deployment for optimal positioning, and cannulation of side-vessels can be performed without (or with minimal) use of x-ray guidance. In one embodiment, guidance can be performed based on OSS-enabled devices, an OSS-enabled stent graft, and a pre-operative CT/live fluoroscopy.

[0029] OSS-enabled devices, such as, e.g., guidewires, catheters etc. provide an operator with knowledge of the shape and deformation and position of points on the device (s) or the entire device(s). The present principles integrate removable optical shape sensed devices into the endograft, stent, balloon, etc. prior to introduction to the body to provide enhanced visualization information during placement. To further provide the operator with knowledge of a deployable device shape, position, and orientation, OSS guidance may be introduced into the deployment process. A deployable or deployment device may include an endograft, stent, guidewire, catheter, balloon catheter, mitral clip, mitral valve, left atrial appendage (LAA) closure device, etc.

[0030] To introduce the use of OSS into an interventional procedure, the fiber needs to be integrated in the device used for the intervention. Incorporating a shape sensing fiber directly into the deployment device may call for the modification of an existing device. One solution includes an optical shape sensing fiber that is integrated into a guidewire used as a 'delivery rail' for the stent deployment system. This guidewire is then registered to the stent or endograft, and then used to model the stent or endograft position and orientation during deployment. Since the deployment device

runs over the guidewire, information about the position and orientation of the device can be obtained; however, information about its state of deployment may not be available. Clipping an OSS enabled retrofit attachment onto the handle of the deployment device can be employed to provide additional information about the state of deployment and thus be used to create a more complete model of the stent or endograft position during deployment. These processes can be complemented through the use of fluoroscopy to update the model.

[0031] It should be understood that the present invention will be described in terms of medical instruments; however, the teachings of the present invention are much broader and are applicable to any fiber optic instruments. In some embodiments, the present principles are employed in tracking or analyzing complex biological or mechanical systems. In particular, the present principles are applicable to internal tracking procedures of biological systems, procedures in all areas of the body such as the lungs, gastro-intestinal tract, excretory organs, blood vessels, etc. The elements depicted in the FIGS. may be implemented in various combinations of hardware and software and provide functions which may be combined in a single element or multiple elements.

[0032] The functions of the various elements shown in the FIGS. can be provided through the use of dedicated hardware as well as hardware capable of executing software in association with appropriate software. When provided by a processor, the functions can be provided by a single dedicated processor, by a single shared processor, or by a plurality of individual processors, some of which can be shared. Moreover, explicit use of the term “processor” or “controller” should not be construed to refer exclusively to hardware capable of executing software, and can implicitly include, without limitation, digital signal processor (“DSP”) hardware, read-only memory (“ROM”) for storing software, random access memory (“RAM”), non-volatile storage, etc.

[0033] Moreover, all statements herein reciting principles, aspects, and embodiments of the invention, as well as specific examples thereof, are intended to encompass both structural and functional equivalents thereof. Additionally, it is intended that such equivalents include both currently known equivalents as well as equivalents developed in the future (i.e., any elements developed that perform the same function, regardless of structure). Thus, for example, it will be appreciated by those skilled in the art that the block diagrams presented herein represent conceptual views of illustrative system components and/or circuitry embodying the principles of the invention. Similarly, it will be appreciated that any flow charts, flow diagrams and the like represent various processes which may be substantially represented in computer readable storage media and so executed by a computer or processor, whether or not such computer or processor is explicitly shown.

[0034] Furthermore, embodiments of the present invention can take the form of a computer program product accessible from a computer-usable or computer-readable storage medium providing program code for use by or in connection with a computer or any instruction execution system. For the purposes of this description, a computer-usable or computer readable storage medium can be any apparatus that may include, store, communicate, propagate, or transport the program for use by or in connection with the instruction execution system, apparatus, or device. The medium can be an electronic, magnetic, optical, electromag-

netic, infrared, or semiconductor system (or apparatus or device) or a propagation medium. Examples of a computer-readable medium include a semiconductor or solid state memory, magnetic tape, a removable computer diskette, a random access memory (RAM), a read-only memory (ROM), a rigid magnetic disk and an optical disk. Current examples of optical disks include compact disk-read only memory (CD-ROM), compact disk-read/write (CD-R/W), Blu-Ray™ and DVD.

[0035] Referring now to the drawings in which like numerals represent the same or similar elements and initially to FIG. 1, a system **100** for tracking and navigation of endografts and related accessories or tools with shape sensing enabled devices and systems is illustratively shown in accordance with one embodiment. The navigation may be manually or robotically performed. System **100** may include a workstation or console **112** from which a procedure is supervised and/or managed. Workstation **112** preferably includes one or more processors **114** and memory **116** for storing programs and applications. Memory **116** may store an optical sensing module **115** configured to interpret optical feedback signals from one or more shape sensing devices or systems **104** (in FIG. 1, the OSS system **104** is located within guidewire **103**, see also FIG. 2). Optical sensing module **115** is configured to use the optical signal feedback (and any other feedback, e.g., electromagnetic (EM) tracking) to reconstruct deformations, deflections and other changes associated with a medical device or instrument, such as an endograft **102** (also referred to herein as a stent graft or stent), one or more guidewires **103** (e.g., a stiff guidewire) which is passed through a deployment device or system **107**, e.g., a commercially available stent deployment system. The deployment system **107** may include a tube or main body **101** through which the guidewire **103** is passed. (See, e.g., cross-section in FIG. 2). The deployment system **107** may include one or more control or stabilizing handles **105** that are employed, depending on the design to perform a plurality of tasks, e.g., to retract a sheath that supports the endograft **102**, to advance a delivery device carrying the endograft **102**, to adjust the guidewire **103** or any other useful function depending on the design of the deployment system **107** and the functions its needs to carry out.

[0036] The shape sensing system **104** includes one or more optical fibers **126** which are included in the system **104** in a set pattern or patterns. The optical fibers **126** connect to the workstation **112**. The shape sensing system **104** may be included in a lumen of the guidewire **103** and/or other medical components involved in the procedure. The OSS fibers **126** or OSS systems **104** are employed to provide a visual representation of the deployable device, such as an endograft or stent. The present principles apply to any use of an optical shape sensing fiber **126** for navigation and deployment of the endograft **102**, or deployment system **107**. While described in terms of the endograft **102**, the present principles can also apply to balloon catheters, clips, valves, and other implantables.

[0037] In one embodiment, the fibers **126** of the OSS system **104** are integrated within or through the guidewire **103**, the deployment system **107** and/or the handle **105** of the deployment system **107**. The OSS system **104** can be employed for making physical measurements. The measurements may be employed for planning or for placement of the

endograft **102**. The endograft **102** may also include an OSS system **104** to provide position and orientation information for the endograft **102** itself.

[0038] Shape sensing system **104** with fiber optics may be based on fiber optic Bragg grating sensors in one or more optical fibers. A fiber optic Bragg grating (FBG) is a short segment of optical fiber that reflects particular wavelengths of light and transmits all others. This is achieved by adding a periodic variation of the refractive index in the fiber core, which generates a wavelength-specific dielectric mirror. A fiber Bragg grating can therefore be used as an inline optical filter to block certain wavelengths, or as a wavelength-specific reflector.

[0039] A fundamental principle behind the operation of a fiber Bragg grating is Fresnel reflection at each of the interfaces where the refractive index is changing. For some wavelengths, the reflected light of the various periods is in phase so that constructive interference exists for reflection and, consequently, destructive interference for transmission. The Bragg wavelength is sensitive to strain as well as to temperature. This means that Bragg gratings can be used as sensing elements in fiber optical sensors. In an FBG sensor, strain causes a shift in the Bragg wavelength.

[0040] One advantage of this technique is that various sensor elements can be distributed over the length of a fiber. Incorporating three or more cores with various sensors (gauges) along the length of a fiber that is embedded in a structure permits a three dimensional form of such a structure to be precisely determined, typically with better than 1 mm accuracy. Along the length of the fiber, at various positions, a multitude of FBG sensors can be located (e.g., 3 or more fiber sensing cores). From the strain measurement of each FBG, the curvature of the structure can be inferred at that position. From the multitude of measured positions, the total three-dimensional form is determined.

[0041] As an alternative to fiber-optic Bragg gratings, the inherent backscatter in conventional optical fiber can be exploited. One such approach is to use Rayleigh scatter in standard single-mode communications fiber. Rayleigh scatter occurs as a result of random fluctuations of the index of refraction in the fiber core. These random fluctuations can be modeled as a Bragg grating with a random variation of amplitude and phase along the grating length. By using this effect in three or more cores running within a single length of multi-core fiber, the 3D shape and dynamics of the surface of interest can be followed.

[0042] It should be understood that optical shape sensing may be performed in a plurality of ways and is not limited to FBGs or Rayleigh scatter techniques. For example, other techniques may include channels etched into the fiber, employing quantum dots for reflection, employing a plurality of separate fibers (e.g., 3 or more) instead of a single multicore fiber or other optical shape sensing techniques.

[0043] Workstation **112** includes a display **118** for viewing internal images of a subject (patient) or volume **131** and may include an image **134** (preoperative or intraoperative images) or an image **136** (OSS data) as an overlay or other rendering registered with the shape sensing system **104** in one or more of the components employed in the procedure. Display **118** may also permit a user to interact with the workstation **112** and its components and functions (e.g., touchscreen, graphical user interface, etc.), or any other element within the system **100**. This is further facilitated by an interface **120** which may include a keyboard, mouse, a

joystick, a haptic device, or any other peripheral or control to permit user feedback from and interaction with the workstation **112**.

[0044] In one embodiment, an OSS fiber **126** or OSS system **104** or OSS enabled device **103**, **105**, **107**, etc. is coupled to the endograft **102**. The OSS fiber **126**, OSS system **104**, etc. is/are registered to a feature or features of the endograft **102**.

[0045] By integrating an OSS enabled device **103**, **105**, **107**, OSS fiber **126** or OSS system **104**, geometric information about the graft **102** may be collected and ultimately used to visualize the graft **102**.

[0046] A registration module **130** is configured to register the OSS fiber **126** or system **104** to a physical structure (e.g., aneurysm, etc.), other OSS systems **104**, images **134**, **136**, the guidewire **103**, the handle **105**, the endograft **102**, etc. For shape recognition registration, a distinctive shape or shape template **128** can be employed to obtain both position and orientation information from the fiber **126**. If the fiber **126** takes a predefined and immutable path, the curvature and shape information of that path can be used to identify a unique image to fiber transformation to be stored in memory **116**.

[0047] An image processing module **142** is configured to combine images (**134**) and OSS position data (image **136**) for joint or separate display on the display **118**. The OSS data **136** and the image data (from pre-operative or intra-operative images **134**) can be registered and jointly displayed to assist in placement of the endograft **102** (or other stent or implantable device). An imaging system **110** may include a fluoroscopy system (x-rays) for collecting real-time visual information about positions of instruments or anatomical features. Images **134** collected with the imaging device **110** may be registered with the OSS data from OSS system **104**.

[0048] One step in endograft **102** deployment is the positioning of x-ray visible (radiopaque) markers **132**. These are initially positioned when the endograft **102** is advanced on the guidewire **103** to the approximate location. If the endograft can be semi-deployed (as in FEVAR), then the markers **132** are re-used to fine tune the position of the endograft **102**. Placement of a three-dimensional endograft **102** within a three-dimensional anatomy is challenging and is typically performed under two-dimensional imaging guidance through x-ray fluoroscopy. As a consequence, misplacement of the endograft **102** can occur, and procedure times can become very long.

[0049] During a conventional FEVAR procedure, a significant portion of time is spent cannulating the fenestrations of an endograft to ensure alignment with an underlying vasculature. Specifically, the operator attempts to align all fenestrations, or windows, to ensure side branches are not occluded by the main stent graft body. The operator must navigate up and into the main stent graft body, then exit the fenestration and enter the side vessel. To do this, the anatomy needs to be seen as well as the position and orientation of the endograft.

[0050] By shape sensing a guidewire **103** and/or a portion of the deployment system **107**, e.g., the handle **105**, and thus the position of the endograft (or at least the relevant markers on the endograft), the navigation can be simplified. Then, navigation can be performed using the registered pre-operative (e.g., CT) images for guidance. To introduce the use of optical shape sensing into an interventional procedure, it is

first necessary to integrate the fiber into one or more of the devices/systems used for the intervention. Given the complexity of these systems, such integration would be both technically challenging and would require significant changes to existing designs. However, by integrating optical shape sensing into the guidewire **103** used during endograft deployment and registering the endograft **102** to the guidewire **103** in accordance with the present principles, the system **100** can be used with any type of stent and/or deployment system **107** with limited impact on design of the endograft or the deployment mechanism.

[0051] In accordance with particularly useful embodiments, the OSS system **104** is integrated into the guidewire **103** over which the endograft deployment system **107** is placed. The deployment system handle **105** is coupled to the guidewire **103** and any motion of the endograft **102** is tracked with respect to the guidewire **103**. The endograft **102** is registered to the OSS system **104** in the guidewire **103**. The guidewire **103** may include a stiff guidewire having diameter of between about 0.014 to about 0.045 inches, and typically about 0.035 inches.

[0052] While the present principles may be applied to any interventional guidewire used in combination with a stent or endograft, the present embodiments employ the guidewire **103** with a lumen or channel therein for OSS system **104** to be disposed so that the position and orientation of the guidewire **103** is known. Such a guidewire **103** acts as a 'delivery rail' for the stent deployment tool (**107**), which passes down a dedicated guidewire lumen within the deployment system **107**. Since the guidewire **103** is physically inside the deployment system **107**, the reconstructed shape of the guidewire **103** is representative of the shape of the deployment system **107**. However, the guidewire **103** is free to rotate and translate inside the deployment system **107**, and therefore, the precise position and orientation of the endograft **102**, x-ray visible markers **132** or the tip of the deployment system **107** may be unknown.

[0053] The configuration of the deployment system **107** is such that one handle **105** may be connected to the endograft **102** in an axially and torsionally stiff manner. This permits re-orientation of the endograft **102** intra-operatively but can also be re-purposed to maintain a registration between the guidewire **103** and the deployment system **107**. This can be achieved in several different ways.

[0054] Referring to FIG. 2, in one embodiment, a clamping mechanism **150** is employed between the guidewire **103** and the deployment system **107**. In cross-sectional view **157**, the guidewire **103** and the deployment system **107** are shown unconstrained. In cross-sectional view **159**, the guidewire **103** and the deployment system **107** are illustratively shown constrained by the clamping mechanism **150**. In this embodiment, the deployment system **107** is advanced over the guidewire **103** until positioned at an approximately correct desired insertion depth. Once at this location, the clamping mechanism **150** within the deployment system **107** would be activated thus physically coupling the deployment system **107** to the guidewire **103**. Thus, pending registration between the OSS system **104** and a known feature in the deployment system **107** (such as x-ray visible markers), any subsequent manipulation of the deployment system **107** is known with respect to a shape sensing co-ordinate system.

[0055] The clamping system **150** may include a system that is integrated into the handle **105** of the deployment device **107** or a retrofit system that attaches to the deploy-

ment system **107** and then clamps the guidewire **103** proximal to entry into the deployment system **107**. The clamping mechanism **150** includes a release **152** to permit clamping and reclamping of the guidewire **103** so that there is still the ability to freely manipulate the guidewire **103**. Alternately, the release **152** may include an actuated release so that the user does not have to apply the clamping force by hand.

[0056] The clamping mechanism **150** may include chucks **151** that compress a tube **101** of the deployment system **107**. The chucks may be hingedly connected and employ one or more pivot axes **155**. The clamping mechanism **150** may be placed at an entry point of the guidewire to the deployment system **107**, although it may also be placed at other locations, e.g., at a point distal to the handle **105** (such as at the tip of the deployment system **107**, within a spindle of the deployment system, or at the proximal position of a loaded stent). Multiple clamping points along the deployment system **107** (such as proximal and distal to the deployment system **107**) may be employed. The OSS system **104** may be fixed within the guidewire lumen at the point of the clamping. This may include a temporary or permanent fixation point.

[0057] It should be understood that the clamping mechanism **150** is merely illustrative of one technique for fastening the guidewire **103** to the deployment system **107** other mechanisms, such as grips, pins, brakes, etc. may also be employed in accordance with the present principles.

[0058] Referring to FIG. 3, a coupling feature **160** may be placed on the guidewire **103** and deployment system **107**. In one embodiment, the guidewire **103** has a predefined coupling feature **160** at a certain location along its length. This could be an adjustable torquer or a more permanent feature bonded to the guidewire **103** at a fixed location. The deployment system **107** also has a coupling feature **162** at the proximal end of the handle **105** such that when both mating features come in contact they engage and rigidly connect the two devices together. Alternatively, the guidewire **103** may clamp onto the handle **105** of the deployment system **107** with no modification to the device handle **105**.

[0059] Where the coupling feature **160** is rigidly fixed to the guidewire **103**, the fixed location could be such that the tip of the guidewire **103** aligns with the tip of the deployment system **107** when the mating components are coupled together, or at any other pre-defined position within or outside the device lumen (**103**). Defining the positioning of this fixed location with respect to the endograft **102** may be part of a pre-registration protocol. In a further embodiment, the coupling of the two devices could take place at the distal tip of the deployment system **107**. View **164** shows the coupling features **160** and **162** prior to engagement, and view **166** shows the coupling features **160** and **162** after engagement.

[0060] Referring to FIG. 4, another embodiment includes a rotational tracking sensor **190** that tracks rotation between the handle **105** and the guidewire **103**. In cases in which it is not desirable to have the guidewire **103** rotationally coupled to the deployment system **107**, it is possible to incorporate sensors **190** into the handle **105** or attachment piece such that the guidewire **103** connects to the deployment system **107** in a manner which enables the relative rotation and translation of the two devices to be measured. This embodiment may include an optical encoder (**190**) (or similar mechanism) within the handle **105** to measure rota-

tion, and a linear potentiometer **191** (or similar mechanism) embedded within the handle **105** but which couples to the guidewire **103**.

[0061] Referring to FIG. 5, another embodiment tracks the handle **105** and the guidewire **103** using a template **192** with the OSS system **104**, using a known shape in the template **192** within the guidewire lumen. If the guidewire **103** is forced to pass through a specific shape within the handle of the deployment system **107**, its position and orientation with respect to the system can be identified.

[0062] Referring to FIG. 6, the endograft **102** may be registered to the guidewire **103** in a number of ways. These may include registering the OSS system **104** in the guidewire **103** to x-ray visible markers **202** on the stent or endograft **102**. This can be performed using an x-ray registration that employs a tip of the guidewire **103** and the markers **202** visible in the x-ray image to determine their relationship. In some cases, the tip of the guidewire **103** may not be visible within the same x-ray image as the stent **102**. An alternative way to perform this registration is to make unique x-ray visible bands **204** on the guidewire **103** along its distal length so that one of those bands is likely to be in close proximity to the endograft or stent **102**, and thus enable registration. Additional methods of registering the OSS system **104** are also contemplated.

[0063] By registering the position of the markers **202** to the guidewire **103** or to markers **204** on the guidewire **103**, a virtual representation of the markers **202**, **204** can be displayed within the 3D visualization framework (e.g., on display **118**, FIG. 1). Then, as the deployment system **107** is manipulated, the position of the markers **202**, **204** can be updated accordingly. Similarly a 3D model of the stent graft **102** can be deformed according to the known positions of the markers **202**, **204** and the OSS shape data from OSS system **104**.

[0064] A 2D overlay of a fluoro image of the stent **102** can be displayed to the user and adapted based on the guidewire position and orientation. This is particularly useful, for example, in FEVAR when the main body stent has been partially deployed and navigation is underway to cannulate the side vessels using OSS-enabled devices. In this situation, knowing the position of the fenestration markers **202** on the stent **102** can provide additional information for navigating through the stent **102** and into side vessels. The stent **102** can be visualized using the information provided by tracking the guidewire **103**.

[0065] It should be noted that in the case of a semi-deployable stent, once the initial position of the stent **102** has been identified and the stent **102** semi-deployed, registration needs to be repeated prior to any further navigation of other OSS enabled devices (catheters guidewires, etc.) through the fenestrations, etc. This is due to the fact that the stent graft **102** will expand and the position of the x-ray visible markers **202** will shift.

[0066] A virtual representation of the stent graft as a full 3D model of the stent may be employed in various stages of deployment. Such a representation would clearly provide a further simplified navigation task. Especially in the case of stenting, where it is important to carefully maintain mechanical properties, it may be preferable to not interfere with the functional properties of the endograft **102**. In addition, there are typically many types of endograft **102** that use only one type of deployment handle **105**. An OSS

system **104** may be employed as a retrofit attachment onto the handle. In this way, multiple stents can be addressed by one design.

[0067] Referring to FIG. 7, another embodiment tracks the handle **105** and the guidewire **103** using a same OSS system **104**. A proximal end of the OSS system **104** exits the guidewire **103** and is connected to a fixed point (attachment point) **174** on the deployment system **107** before returning to a launch fixture **170**. As before, the location of this fixed point **174** is preferably on the distal handle **105** of the deployment system **107** since this is rigidly coupled to a main backbone of the system **107** and thus the location of the endograft **102**.

[0068] Referring to FIG. 8, another embodiment tracks the handle **105** and the guidewire **103** using different OSS systems **104**. A second OSS system **104'** is attached to a fixed point **184** on the deployment system **107** and registered to a shape sensing co-ordinate system. The location of this fixed point **184** is preferably at a point on the handle **105** of the deployment system **107** since this is rigidly coupled to a main backbone of the system **107** and thus the location of the endograft **102**. This configuration permits the guidewire **103** to be rotated and translated with respect to the deployment system **107**.

[0069] Referring to FIG. 9, four positions **210**, **212**, **214** and **216** of a deployment system are depicted with corresponding model images **220**, **222**, **224** and **226** of blood vessels having a stent **102** being deployed therein, are depicted. A clip-on attachment **302** (or set of attachments) may be included to connect one or more OSS systems **104** to a handle or handles **105** of the deployment system **107**. A method for registering the stent **102** to the OSS system **104** is also needed. The clip-on attachment **302** that connects to the deployment system **107** can provide a simple way to enable visualization of the endograft deployment process. Motions at a proximal portion of the deployment system **107** directly map to changes in the stent position and state of deployment.

[0070] In one embodiment, the clip-on attachment **302** includes adhesive strips or pieces that are employed that attach to the OSS system **104** and are fixed to the proximal and distal handles **105** of the deployment system **107**. The OSS system **104** returns back to a launch base or fixture **308** where its origin resides. Clips **302** can be removed and re-applied for another stent deployment within a same procedure. The clips **302** can be comprised of a mechanical fixation device (e.g., clip, toggle clamp, spring clasp, etc.), an adhesive, a magnetic attachment, a band or other attachment device.

[0071] The position of the stent graft **102**, the orientation of the stent graft **102** and the state of deployment (how many of the individual stents on the stent graft have been deployed) need to be known. There are three primary features that need be known about the stent to provide a meaningful visualization. It is assumed that a shape sensed guidewire **103** is being used as part of the deployment process. This guidewire **103** can provide part of the information to determine the position of the stent **102**. In some cases, the guidewire **103** may not be coupled to the deployment system **107** so it does not provide information about the orientation. The clip-on attachment **302** can sense the orientation of a retaining ring of the stent graft **102** (or whichever portion of the stent graft that is rigidly attached to the deployment system **107**) because the orientation of the

distal portion of the handle **105** is directly coupled to the orientation of the attachment site of the stent graft **102** (very stiff torsionally). This is what enables the fine manipulation of the stent graft **102** during deployment. Therefore, by sensing the position of the distal deployment handle **105**, the orientation of the attachment point on the stent graft **102** can be extracted.

[0072] The clip-on attachment **302** may provide information about the state of deployment of the stent graft **102** by measuring a relative position of actuating elements (e.g., handles **105**) of the stent deployment system **107**. As shown in FIG. 9, separation between the distal and proximal handles **105** on the deployment system directly relates to how many individual stents or stent length that has been released. Visualization of the stent deployment using shape sensing on the handles **105** with a clip-on attachment **302** includes OSS system **104** attached to both distal and proximal handles.

[0073] It would also be possible to infer the state of stent deployment by incorporating the OSS system **104** into the handle or handles **105** of the deployment system **107** without modification of the multiple different deployment systems available on the market. Interfacing of the OSS system(s) **104** can be done with a separate OSS visualization framework. The clip-on attachment **302** provides the same functionality as the embodiments described above without the need for handle modifications. The clip-on attachment **302** to the handle **105** can be done with a different OSS system **104** than that employed for the guidewire **103**, or by using the OSS system **104** after leaving from a proximal portion of the guidewire **103**.

[0074] Referring to FIG. 10, an illustrative deployment system **107** is shown along with a magnified view of an adhesive clip-on attachment **302'**. In addition to attaching onto the handle **105**, the adhesive or clip attachment **302'** can also be used to sense a distal portion of the deployment system **107**. This clip **302'** may include an adhesive attachment or patch **312** that couples the OSS system **104** to the outside of the deployment system **107**. This adhesive patch **312** can also have a radiopaque marker **314** integrated into it for registration purposes. The OSS system **104** travels back from the deployment system **107** to a launch fixture **308** outside the body. Alternatively, it could travel back to an attachment point on the handle **105**.

[0075] Once the clip-on attachment **302**, **302'** has been fixed to the deployment system **107**, it may not be necessary to register the endograft **102** to the deployment system **107** if the stent **102** is incorporated into the deployment system **107** in the same way each time for a given stent deployment product. However, it is likely that it will be necessary to register each stent to the deployment system **107** prior to use.

[0076] There is a very torsionally stiff relationship between the stent anchor (e.g., anchor ring) and the handle **105**, which is what gives the handle **105** the ability to re-orient the stent **102** during deployment. The more important registration is in orientation. This relationship will likely vary in each stent **102**. For this reason, the Information for Use (IFU) for each stent **102** includes a step at the beginning of the process where the stent **102** is visualized under x-ray by the operator, rotated based on the x-ray visible markers (**202**) present, and then mentally mapped to an indicator **322** on the handle **105** so as to remember an 'optimal' orientation for deployment. After navigating, the operator then returns

the handle **105** to the optimal orientation (as indicated by a recalled position of the dot **322**). This same procedure can be used following attachment of the OSS system **104**. For example, the stent **102** is rotated until it is fully in plane (based on the marker bands **202**) and then that position is used to map the OSS system **104** to the stent **102** in orientation. This could be done manually or robotically.

[0077] The next important registration is in position. This is principally the distance along the deployment system **107** between the stent **102** and the OSS clip **302** onto the handle **105**. Specifically, the position of the x-ray visible markers (**202**) within the stent **102** should be known. This distance can be identified using a multitude of different methods. For example, one embodiment would include a priori knowledge of the mechanical construction of the stent deployment system **107**. Another embodiment includes determining the distance under x-ray guidance. If the shape sensing base is registered to the x-ray system then the stent deployment system **107** can be placed straight and with the stent visible under x-ray. The marker bands (**204**) can be selected in the image and then the distance between the clips (**302**) on the handle (**105**) and the marker bands will be known. This can be done prior to deployment as the marker bands are visible at that time. Another embodiment employs an x-ray image of the stent deployment system **107** that can be used to identify the offset between the deployment system tip and the marker bands (**204**) on the stent graft **102**. From the known orientation, position, and state of deployment, a model of the endograft can be generated and displayed to the user.

[0078] The present principles can be applied to any use of an optical shape sensing fiber or system for navigation and deployment of a stent, stent-graft, or stent deployment system. The present principles can also be applied to any stent and balloon, i.e., to any over the wire therapy device, to track the position of the device in the vessel, to help position the device and deliver therapy with less x-ray and less contrast media volume. In such embodiments, a stiff guidewire would likely be replaced by a more flexible wire, either or both may be OSS tracked.

[0079] It should be understood that the present principles cover any of the applications where an endograft is deployed under fluoroscopic or other guidance including, but not limited to procedures, such as, e.g., endovascular aneurysm repair (EVAR), branch-fenestrated EVAR (BEVAR), percutaneous EVAR (PEVAR), thoracic EVAR (TEVAR), fenestrated EVAR (FEVAR), etc.

[0080] Referring to FIG. 11, a method for endograft deployment is described and shown in accordance with illustrative embodiments. In block **402**, a guide wire having an optical shape sensing (OSS) system within a lumen of the guide wire is deployed. The guide wire is configured to deliver an endograft into a vessel. The guide wire may be disposed within a deployment system or tool. The deployment system or tool may have relative motion (e.g., free rotation, measured rotation, etc.) with respect to the guidewire or the relative motion may be constrained. The deployment system and the guidewire may be clamped together or coupled together when engaging at a particular point, etc.

[0081] In block **408**, the OSS system may be attached to the at least one handle or deployment system using a clip-on attachment device or other means. In one embodiment, the deployment system may include two handles and the OSS

system may be attached between the two handles to measure relative distance between the handles using the OSS system.

[0082] In block **410**, shape, position and/or orientation of the guide wire are measured using the OSS system to identify a shape, position and orientation of the endograft during deployment. The shape, position and/or orientation of the handle may be measured with the OSS system inside the guide wire or may be measured using an additional OSS system.

[0083] In block **412**, the endograft is registered with OSS data and/or with image data of the vessel where the endograft is placed. In block **413**, the guidewire may be clamped or coupled to the deployment system to prevent relative motion therebetween. The deployment system may include at least one handle. The OSS system may also be coupled to the at least one handle. In block **414**, the endograft is registered with the guide wire using one or more radiopaque markers along a length of the guidewire and/or on the endograft. In block **416**, the guidewire may include a shape template and the OSS data is registered to the image data using the shape template. The shape template includes a distinctive shape that can be matched between OSS data and image data to register one or more of the deployment system, the guidewire, the stent, etc.

[0084] In block **418**, the endograft is anchored in the blood vessel. In block **420**, the guidewire and the OSS system are removed from the vessel.

[0085] In interpreting the appended claims, it should be understood that:

[0086] a) the word “comprising” does not exclude the presence of other elements or acts than those listed in a given claim;

[0087] b) the word “a” or “an” preceding an element does not exclude the presence of a plurality of such elements;

[0088] c) any reference signs in the claims do not limit their scope;

[0089] d) several “means” may be represented by the same item or hardware or software implemented structure or function; and

[0090] e) no specific sequence of acts is intended to be required unless specifically indicated.

[0091] Having described preferred embodiments for device visualization through optical shape sensing of a guidewire (which are intended to be illustrative and not limiting), it is noted that modifications and variations can be made by persons skilled in the art in light of the above teachings. It is therefore to be understood that changes may be made in the particular embodiments of the disclosure disclosed which are within the scope of the embodiments disclosed herein as outlined by the appended claims. Having thus described the details and particularity required by the patent laws, what is claimed and desired protected by Letters Patent is set forth in the appended claims.

1. A medical device deployment system, comprising:
 - a main body;
 - a guidewire capable of being passed through the main body and including a lumen; and
 - an optical shape sensing (OSS) system comprising an optical fiber, which comprises a fiber Bragg grating sensor, the OSS system being configured to pass through the lumen in the guidewire, the OSS system being configured to measure at least one of shape, position or orientation of a medical device being

deployed relative to an anatomical feature and output optical shape sensing data obtained from reflections within the optical fiber of the OSS system indicative of a shape of the optical fiber, wherein: the guidewire is centrally located in the main body; and the OSS system is centrally located in the lumen of the guidewire.

2. The deployment system as recited in claim 1, wherein the guidewire is deformed with a shape template for registering the position in the optical shape sensing data along the guidewire.

3. The deployment system as recited in claim 1, further comprising at least one handle coupled to the main body, the at least one handle including an attachment position for the OSS system exiting the guidewire.

4. The deployment system as recited in claim 1, further comprising at least one handle coupled to the main body, the at least one handle including an attachment position for an additional OSS system.

5. The deployment system as recited in claim 1, further comprising a clamping mechanism configured to clamp the main body to the guidewire.

6. The deployment system as recited in claim 1, further comprising a first coupling feature on the main body and a second coupling feature on the guidewire, the first coupling feature and the second coupling feature being configured to engage each other to connect to prevent relative motion therebetween.

7. The deployment system as recited in claim 1, further comprising a rotation tracking sensor configured to measure rotation between the main body and the guidewire.

8. The deployment system as recited in claim 1, further comprising an endograft; and radiopaque markers disposed on the guidewire to permit registration between the guidewire and the endograft.

9. The deployment system as recited in claim 1, further comprising at least one clip-on attachment configured to attach the OSS system to a control handle of the deployment system, wherein the at least one clip-on attachment includes an adhesive portion coupled to the deployment system to attach the OSS system, the adhesive portion including a radiopaque feature.

10. The deployment system as recited in claim 1, wherein the deployment system is an endograft deployment system or is a deployment system which includes a mitral clip, a valve or a balloon catheter.

11. An endograft deployment system, comprising:

- a workstation including a processor;
- a tangible, non-transitory computer readable medium that stores executable instructions, which when executed by the processor, cause the processor to: interpret optical shape sensing data; and register the optical shape sensing data to pre-operative or intra-operative images;
- a deployment system including a tube;
- a guidewire capable of being passed through the tube, the guidewire including a lumen;
- an optical shape sensing (OSS) system comprising an optical fiber, which comprises a fiber Bragg grating sensor, the OSS system being configured to pass through the lumen in the guidewire, the OSS system being configured to measure at least one of shape, position or orientation of an endograft relative to a blood vessel for placement of the endograft to provide the optical shape sensing data wherein: the

guidewire is centrally located in the tube; and the OSS system is centrally located in the lumen of the guidewire.

12. The endograft deployment system as recited in claim **11**, wherein the guidewire is deformed with a shape template for registering the position in shape data along the guidewire.

13. The endograft deployment system as recited in claim **11**, further comprising at least one handle coupled to the tube, the at least one handle including an attachment position for the OSS system exiting the guidewire.

14. The endograft deployment system as recited in claim **11**, further comprising at least one handle coupled to the tube, the at least one handle including an attachment position for an additional OSS system.

15. The endograft deployment system as recited in claim **11**, further comprising:

a clamping mechanism configured to clamp the tube to the guidewire;

a first coupling feature on the tube and a second coupling feature on the guidewire, the first coupling feature and the second coupling feature being configured to engage each other to connect to prevent relative motion therebetween;

a rotation tracking sensor configured to measure rotation between the tube and the guidewire;

radiopaque markers disposed on the guidewire to permit registration between the guidewire and the endograft; and

at least one clip-on attachment configured to attach the OSS system to a control handle of the deployment system,

wherein the at least one clip-on attachment includes an adhesive portion coupled to the deployment system to attach the OSS system, the adhesive portion including a radiopaque feature.

16. A method for endograft deployment, comprising:

deploying a guidewire having an optical shape sensing (OSS) system within a lumen of a guide wire, the guide wire configured to deliver an endograft into a vessel, wherein: the guidewire is centrally located in a tube; and the OSS system is centrally located in the lumen of the guidewire;

measuring at least one of shape, position or orientation of the guide wire using the OSS system to identify a shape, position or orientation of the endograft during deployment;

registering OSS data with image data on the vessel where the endograft is placed;

anchoring the endograft in a blood vessel; and

removing the guidewire and the OSS system from the vessel.

17. The method as recited in claim **16**, wherein deploying includes using a deployment system having at least one handle, the OSS system being coupled to the at least one handle and the method further comprises:

measuring the at least one of shape, position or orientation of the handle along with the guide wire.

18. The method as recited in claim **16**, further comprising attaching (408) the OSS system to at least one handle using a clip-on attachment device.

19. The method as recited in claim **16**, wherein registering OSS data with image data on the vessel includes registering the endograft with the guidewire using one or more radiopaque markers along a length of the guidewire.

20. The method as recited in claim **16**, wherein the guidewire is deformed by a shape template and the step of registering includes registering the OSS data to the image data using the shape template.

* * * * *