



US007150749B2

(12) **United States Patent**
Dycus et al.

(10) **Patent No.:** **US 7,150,749 B2**
(45) **Date of Patent:** **Dec. 19, 2006**

(54) **VESSEL SEALER AND DIVIDER HAVING ELONGATED KNIFE STROKE AND SAFETY CUTTING MECHANISM**

2,632,661 A	3/1953	Cristofv
2,668,538 A	2/1954	Baker
2,796,065 A	6/1957	Kapp
3,459,187 A	8/1969	Pallotta
3,643,663 A	2/1972	Sutter
3,651,811 A	3/1972	Hildebrandt et al.
3,862,630 A	1/1975	Balamuth
3,866,610 A	2/1975	Kletschka

(75) Inventors: **Sean T. Dycus**, Denver, CO (US);
Duane E. Kerr, Berthoud, CO (US);
Darion Peterson, Boulder, CO (US)

(73) Assignee: **Sherwood Services AG**, Schaffhausen (CH)

(Continued)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

FOREIGN PATENT DOCUMENTS

CA 2104423 2/1994

(Continued)

(21) Appl. No.: **10/953,757**

OTHER PUBLICATIONS

(22) Filed: **Sep. 29, 2004**

Sigel et al. "The Mechanism of Blood Vessel Closure by High Frequency Electrocoagulation" Surgery Gynecology & Obstetrics, Oct. 1965 pp. 823-831.

(65) **Prior Publication Data**

US 2005/0107785 A1 May 19, 2005

(Continued)

Related U.S. Application Data

Primary Examiner—Henry M. Johnson, III

(63) Continuation-in-part of application No. 10/460,926, filed on Jun. 13, 2003.

(57)

ABSTRACT

(51) **Int. Cl.**

A61B 18/12 (2006.01)

(52) **U.S. Cl.** **606/51**; 606/32; 606/41

(58) **Field of Classification Search** 606/32–52
See application file for complete search history.


An endoscopic bipolar forceps includes a housing and a shaft affixed to the housing. The shaft includes a longitudinal axis defined therethrough and a pair of jaw members attached to a distal end thereof. The forceps also includes a drive assembly for moving one of the jaw members relative to the other jaw member. A movable handle is included which moves the jaw members from the open and closed positions. The forceps is adapted to connect to a source of electrosurgical energy such that the jaw members are capable of conducting bipolar energy through tissue held therebetween to effect a tissue seal. A trigger assembly is operatively disposed relative to the movable handle for selectively advancing a knife assembly for cutting tissue along the tissue seal. The knife assembly includes a knife collar which cooperates with a knife shaft to advance a knife through tissue upon activation of the trigger assembly.

(56) **References Cited**

U.S. PATENT DOCUMENTS

371,664 A	10/1887	Brannan et al.
702,472 A	6/1902	Pignolet
728,883 A	5/1903	Downes
1,586,645 A	6/1926	Bierman
2,002,594 A	5/1935	Wappler et al.
2,011,169 A	8/1935	Wappler
2,031,682 A	2/1936	Wappler et al.
2,176,479 A	10/1939	Willis
2,305,156 A	12/1942	Grubel

4 Claims, 27 Drawing Sheets

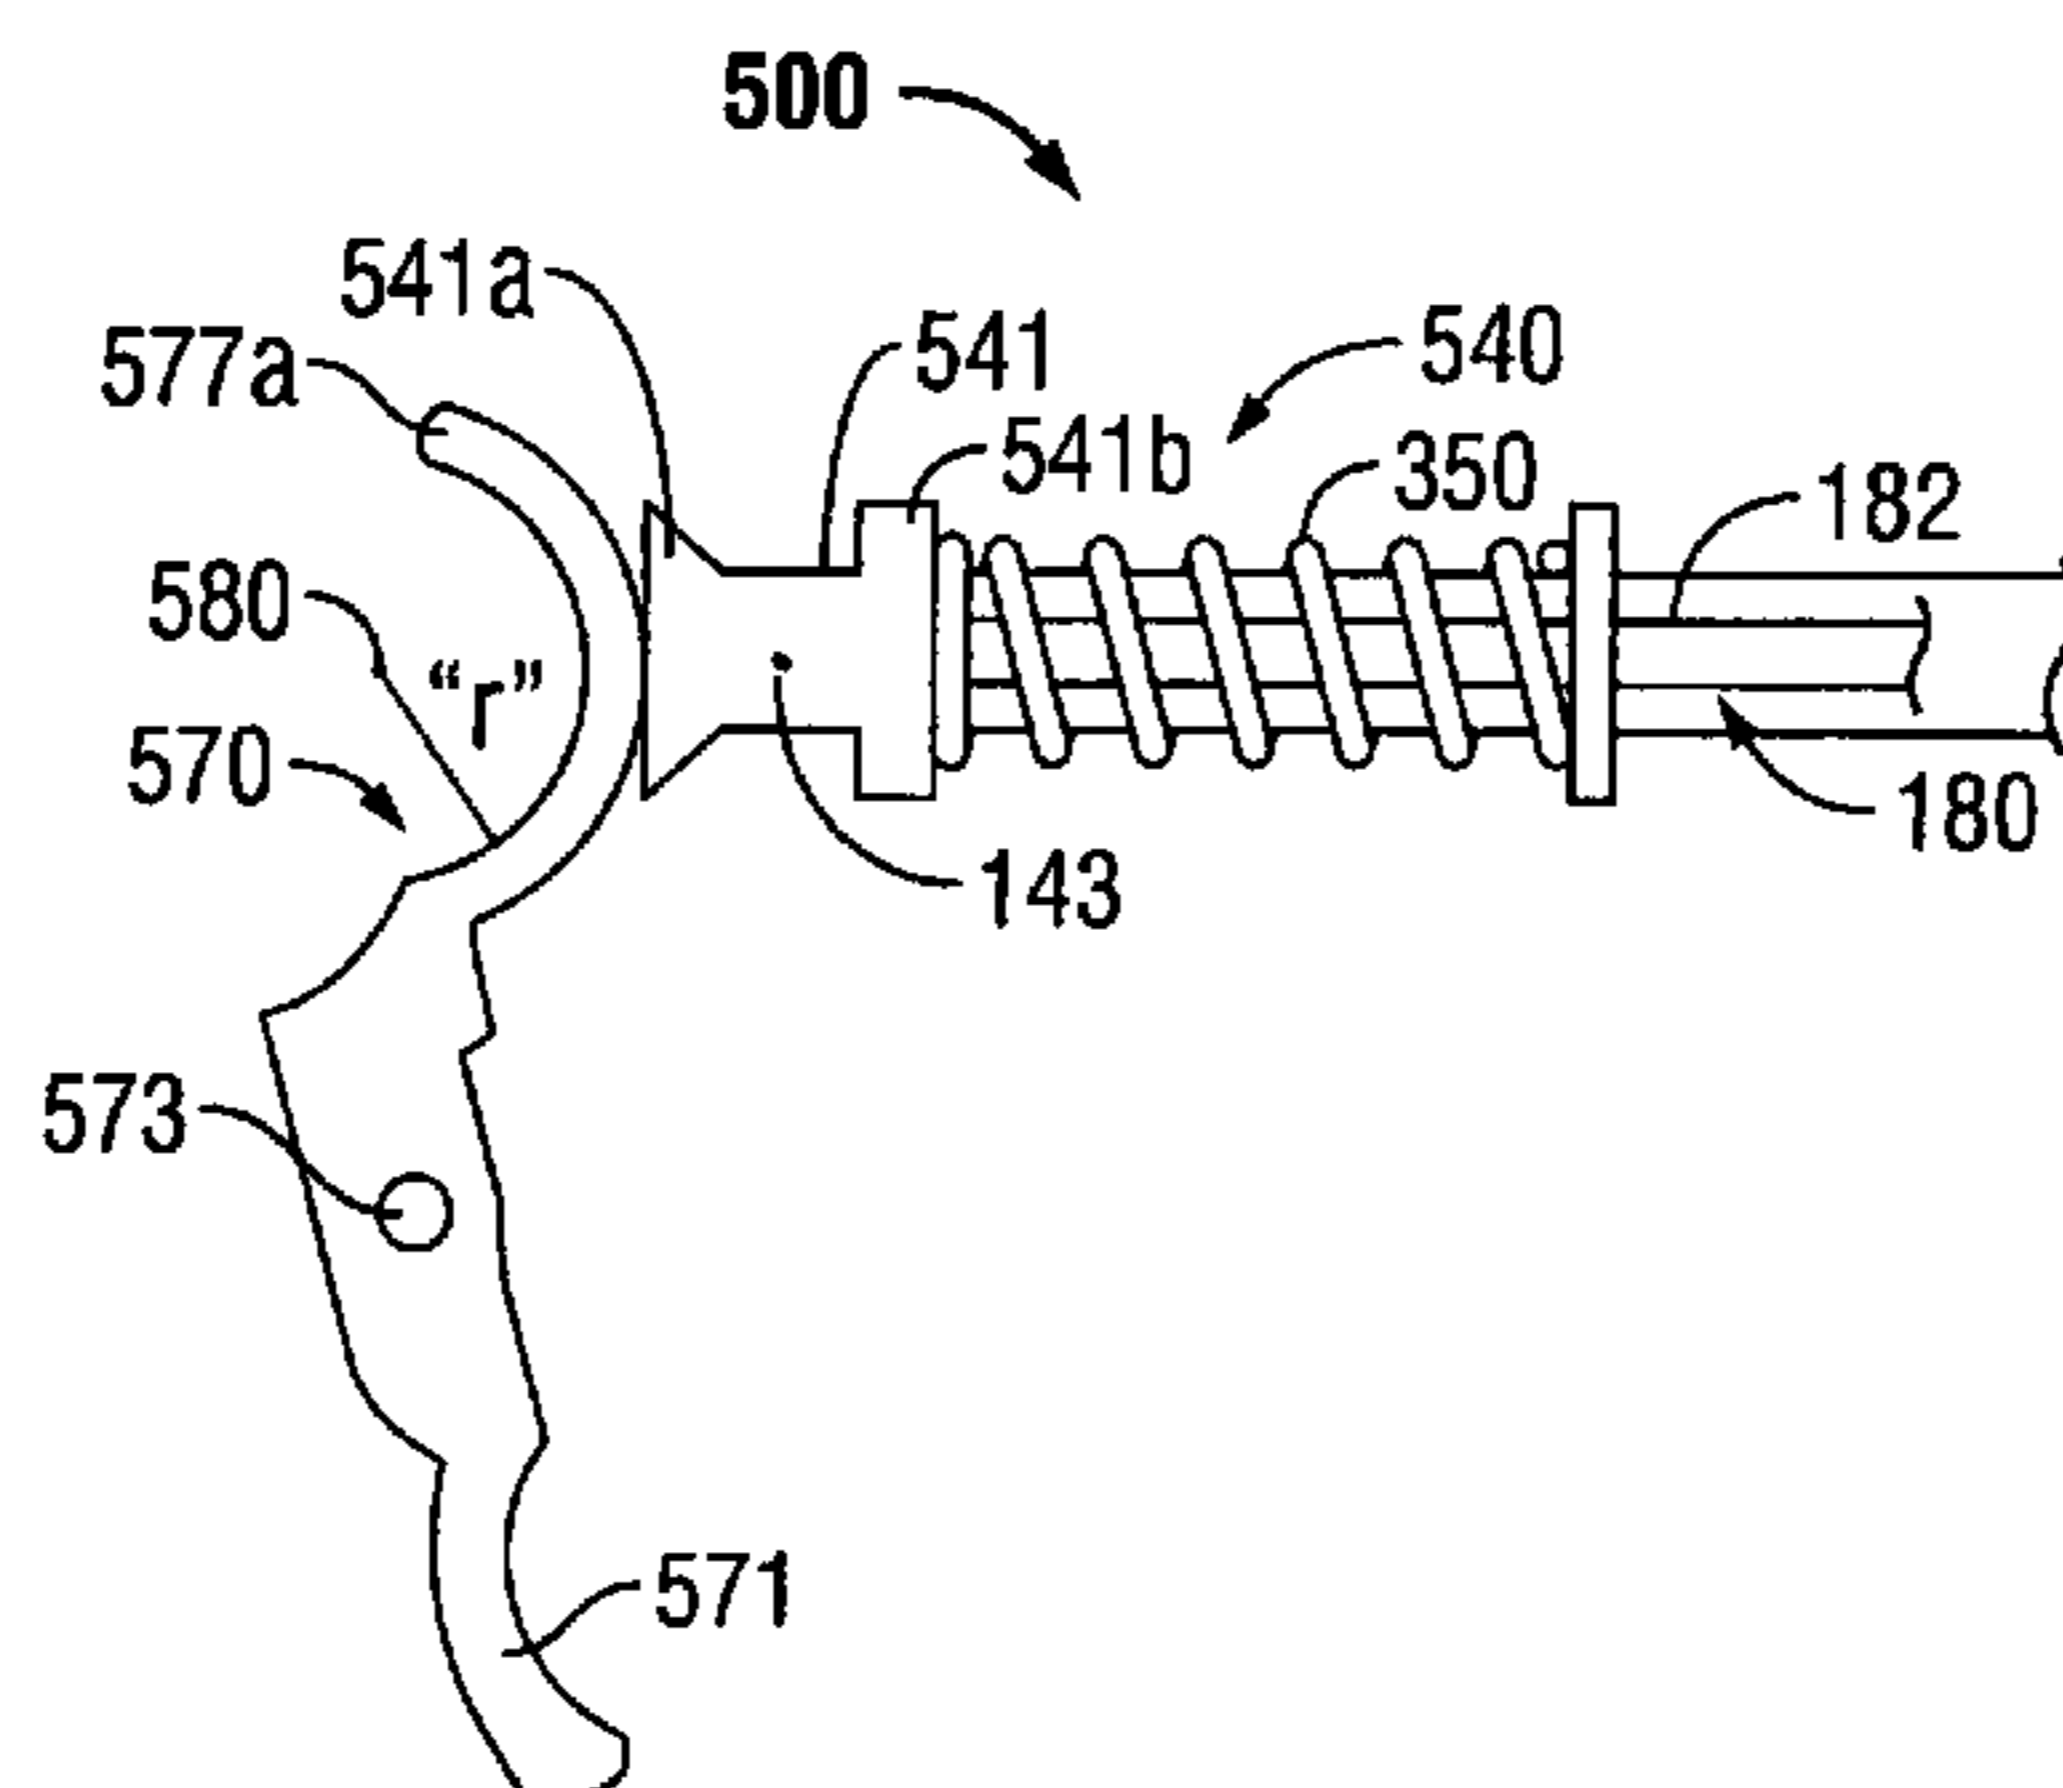

US 7,150,749 B2

Page 2

U.S. PATENT DOCUMENTS			
		5,415,657 A	5/1995 Taymor-Luria
		5,422,567 A	6/1995 Matsunaga
		5,423,810 A	6/1995 Goble et al.
		5,425,739 A	6/1995 Jessen
		5,429,616 A	7/1995 Schaffer
		5,431,674 A	7/1995 Basile et al.
		5,437,292 A	8/1995 Kipshidze et al.
		5,438,302 A	8/1995 Goble
		5,441,517 A	8/1995 Kensey et al.
		5,443,463 A	8/1995 Stern et al.
		5,443,464 A	8/1995 Russell et al.
		5,443,480 A	8/1995 Jacobs et al.
		5,445,638 A	8/1995 Rydell et al.
		5,445,658 A	8/1995 Durrfeld et al.
		5,451,224 A	9/1995 Goble et al.
		5,456,684 A	10/1995 Schmidt et al.
		5,458,598 A	10/1995 Feinberg et al.
		5,460,629 A	10/1995 Shlain et al.
		5,462,546 A	10/1995 Rydell
		5,472,443 A	12/1995 Cordis et al.
		5,478,351 A	12/1995 Meade et al.
		5,484,436 A	1/1996 Eggers et al.
		5,496,317 A	3/1996 Goble et al.
		5,499,997 A	3/1996 Sharpe et al.
		5,509,922 A	4/1996 Aranyi et al.
		5,514,134 A	5/1996 Rydell et al.
		5,527,313 A	6/1996 Scott et al.
		5,531,744 A	7/1996 Nardella et al.
		5,536,251 A	7/1996 Evard et al.
		5,540,684 A	7/1996 Hassler, Jr.
		5,540,685 A	7/1996 Parins et al.
		5,540,715 A	7/1996 Katsaros et al.
		5,558,672 A	9/1996 Edwards et al.
		5,569,241 A	10/1996 Edwardds
		5,569,243 A	10/1996 Kortenbach et al.
		5,571,100 A	11/1996 Goble et al.
		5,573,424 A	11/1996 Poppe
		5,573,535 A	11/1996 Viklund
		5,582,611 A	12/1996 Tsukagoshi et al.
		5,585,896 A	12/1996 Yamazaki et al.
		5,590,570 A	1/1997 LeMaire, III et al.
		5,603,711 A	2/1997 Parins et al.
		5,603,723 A	2/1997 Aranyi et al.
		5,626,578 A	5/1997 Tihon
		5,626,609 A	5/1997 Zvenyatsky et al.
		5,630,833 A	5/1997 Katsaros et al.
		5,637,110 A	6/1997 Pennybacker et al.
		5,643,294 A	7/1997 Tovey et al.
		5,647,869 A	7/1997 Goble et al.
		5,647,871 A	7/1997 Levine et al.
		5,649,959 A	7/1997 Hannam et al.
		5,658,281 A	8/1997 Heard
		5,662,667 A	9/1997 Knodel
		5,667,526 A	9/1997 Levin
		5,674,220 A	10/1997 Fox et al.
		5,693,051 A	12/1997 Schulze et al.
		5,695,522 A	12/1997 LeMaire, III et al.
		5,700,261 A	12/1997 Brinkerhoff
		5,702,390 A	12/1997 Austin et al.
		5,707,369 A	1/1998 Vaitekunas et al.
		5,709,680 A	1/1998 Yates et al.
		5,716,366 A	2/1998 Yates
		5,720,744 A	2/1998 Eggleston et al.
		5,727,428 A	3/1998 LeMaire, III et al.
		5,735,848 A	4/1998 Yates et al.
		5,743,906 A	4/1998 Parins et al.
		5,755,717 A	5/1998 Yates et al.
		5,766,130 A	6/1998 Selmonosky
		5,766,166 A	6/1998 Hooven
		5,766,170 A	6/1998 Eggers
		5,769,849 A	6/1998 Eggers
		5,776,128 A	7/1998 Eggers
		5,776,130 A	7/1998 Buysse et al.
3,911,766 A	10/1975		Fridolph et al.
3,920,021 A	11/1975		Hiltebrandt
3,921,641 A	11/1975		Hulka
3,938,527 A	2/1976		Rioux et al.
3,952,749 A	4/1976		Fridolph et al.
4,005,714 A	2/1977		Hiltebrandt
4,074,718 A	2/1978		Morrison, Jr.
4,088,134 A	5/1978		Mazzariello
4,165,746 A	8/1979		Burgin
4,300,564 A	11/1981		Furihata
4,370,980 A	2/1983		Lottick
4,452,246 A	6/1984		Bader et al.
4,492,231 A	1/1985		Auth
4,552,143 A	11/1985		Lottick
4,574,804 A	3/1986		Kurwa
4,597,379 A	7/1986		Kihn et al.
4,600,007 A	7/1986		Lahodny et al.
4,657,016 A	4/1987		Garito et al.
4,662,372 A	5/1987		Sharkany et al.
4,671,274 A	6/1987		Sorochenko
4,685,459 A	8/1987		Koch et al.
D295,893 S	5/1988		Sharkany et al.
D295,894 S	5/1988		Sharkany et al.
4,763,669 A	8/1988		Jaeger
4,827,929 A	5/1989		Hodge
4,887,612 A	12/1989		Esser et al.
4,938,761 A	7/1990		Ensslin
4,985,030 A	1/1991		Melzer et al.
5,007,908 A	4/1991		Rydell
5,026,370 A	6/1991		Lottick
5,099,840 A	3/1992		Goble et al.
5,116,332 A	5/1992		Lottick
5,147,357 A	9/1992		Rose et al.
5,151,102 A	9/1992		Kamiyama et al.
5,176,695 A	1/1993		Dulebohn
5,197,964 A	3/1993		Parins
5,215,101 A	6/1993		Jacobs et al.
5,217,457 A	6/1993		Delahuerga et al.
5,217,458 A	6/1993		Parins
5,244,462 A	9/1993		Delahuerga et al.
5,250,047 A	10/1993		Rydell
5,258,006 A	11/1993		Rydell et al.
5,261,918 A	11/1993		Phillips et al.
5,275,615 A	1/1994		Rose
5,277,201 A	1/1994		Stern
5,282,799 A	2/1994		Rydell
5,290,286 A	3/1994		Parins
5,304,203 A	4/1994		El-Mallawany et al.
5,308,357 A	5/1994		Lichtman
5,318,589 A	6/1994		Lichtman
5,324,289 A	6/1994		Eggers
5,330,471 A	7/1994		Eggers
5,334,183 A	8/1994		Wuchinich
5,334,215 A	8/1994		Chen
5,336,221 A	8/1994		Anderson
5,342,359 A	8/1994		Rydell
5,342,381 A	8/1994		Tidemand
5,342,393 A	8/1994		Stack
5,352,222 A	10/1994		Rydell
5,354,271 A	10/1994		Voda
5,356,408 A	10/1994		Rydell
5,366,477 A	11/1994		LeMarie, III et al.
5,383,897 A	1/1995		Wholey
5,389,098 A	2/1995		Tsuruta et al.
5,389,104 A	2/1995		Hahnen et al.
5,391,166 A	2/1995		Eggers
5,391,183 A	2/1995		Janzen et al.
5,403,312 A	4/1995		Yates et al.
5,411,519 A	5/1995		Tovey et al.
5,411,520 A	5/1995		Nash et al.
5,413,571 A	5/1995		Katsaros et al.

US 7,150,749 B2

5,779,701 A	7/1998	McBrayer et al.	6,277,117 B1	8/2001	Tetzlaff et al.
5,792,137 A	8/1998	Carr et al.	6,280,458 B1	8/2001	Boche et al.
5,792,177 A	8/1998	Kaseda	6,283,961 B1	9/2001	Underwood et al.
5,797,927 A *	8/1998	Yoon 606/144	D449,886 S	10/2001	Tetzlaff et al.
5,797,938 A	8/1998	Paraschac et al.	6,322,561 B1	11/2001	Eggers et al.
5,797,958 A	8/1998	Yoon	6,334,860 B1	1/2002	Dorn
5,800,449 A	9/1998	Wales	6,334,861 B1	1/2002	Chandler et al.
5,810,808 A	9/1998	Eggers	6,350,264 B1	2/2002	Hooven
5,810,811 A	9/1998	Yates et al.	6,352,536 B1	3/2002	Buysse et al.
5,814,043 A	9/1998	Shapeton	D457,958 S	5/2002	Dycus et al.
5,817,083 A	10/1998	Williamson, IV et al.	D457,959 S	5/2002	Tetzlaff et al.
5,820,630 A	10/1998	Lind	6,398,779 B1	6/2002	Buysse et al.
5,827,271 A	10/1998	Buysse et al.	6,409,728 B1	6/2002	Ehr et al.
5,827,279 A	10/1998	Hughett et al.	6,419,675 B1	7/2002	Gallo, Sr.
5,827,281 A	10/1998	Levin	6,425,896 B1	7/2002	Baltschun et al.
5,833,690 A	11/1998	Yates et al.	6,440,144 B1	8/2002	Bacher
5,843,080 A	12/1998	Fleenor et al.	6,443,970 B1	9/2002	Schulze et al.
5,849,022 A	12/1998	Sakashita et al.	6,451,018 B1	9/2002	Lands et al.
5,853,412 A	12/1998	Mayenberger	6,458,128 B1	10/2002	Schulze
5,876,401 A	3/1999	Schulze et al.	6,458,130 B1	10/2002	Frazier et al.
5,891,141 A	4/1999	Rydell	6,464,702 B1	10/2002	Schulze et al.
5,891,142 A	4/1999	Eggers et al.	6,464,704 B1	10/2002	Schmaltz et al.
5,893,863 A	4/1999	Yoon	6,511,480 B1	1/2003	Tetzlaff et al.
5,893,875 A	4/1999	O'Connor et al.	6,585,735 B1	7/2003	Frazier et al.
5,902,301 A	5/1999	Olig	6,620,161 B1	9/2003	Schulze et al.
5,906,630 A	5/1999	Anderhub et al.	6,626,901 B1	9/2003	Treat et al.
5,908,420 A	6/1999	Parins et al.	6,682,528 B1	1/2004	Frazier et al.
5,913,874 A	6/1999	Berns et al.	6,695,840 B1	2/2004	Schulze
5,921,984 A	7/1999	Sutcu et al.	6,726,686 B1	4/2004	Buysse et al.
5,935,126 A	8/1999	Riza	6,743,229 B1	6/2004	Buysse et al.
5,944,718 A	8/1999	Dafforn et al.	6,770,072 B1	8/2004	Truckai et al.
5,951,549 A	9/1999	Richardson et al.	D496,997 S	10/2004	Dycus et al.
5,954,720 A	9/1999	Wilson et al.	D499,181 S	11/2004	Dycus et al.
5,976,132 A	11/1999	Morris	2002/0188294 A1	12/2002	Couture et al.
5,989,277 A	11/1999	LeMaire, III et al.	2003/0014052 A1	1/2003	Buysse et al.
6,004,335 A	12/1999	Vaitekunas et al.	2003/0014053 A1	1/2003	Nguyen et al.
6,010,516 A	1/2000	Hulka	2003/0018331 A1	1/2003	Dycus et al.
6,024,741 A	2/2000	Williamson et al.	2003/0018332 A1	1/2003	Schmaltz et al.
6,024,744 A	2/2000	Kese et al.	2003/0032956 A1	2/2003	Lands et al.
6,033,399 A	3/2000	Gines	2003/0069571 A1	4/2003	Treat et al.
6,039,733 A	3/2000	Buysse et al.	2003/0109875 A1	6/2003	Tetzlaff et al.
6,041,679 A	3/2000	Slater et al.	2003/0139742 A1	7/2003	Wampler et al.
6,050,996 A	4/2000	Schmaltz et al.	2003/0158549 A1	8/2003	Swanson
6,053,914 A	4/2000	Eggers et al.	2003/0181910 A1	9/2003	Dycus et al.
6,053,933 A	4/2000	Balazs et al.	2003/0199869 A1	10/2003	Johnson et al.
D424,694 S	5/2000	Tetzlaff et al.	2003/0229344 A1	12/2003	Dycus et al.
D425,201 S	5/2000	Tetzlaff et al.	2004/0082952 A1	4/2004	Dycus et al.
RE36,795 E	7/2000	Rydell	2004/0087943 A1	5/2004	Dycus et al.
6,083,223 A	7/2000	Baker	2004/0115296 A1	6/2004	Duffin
6,086,586 A	7/2000	Hooven	2004/0116924 A1	6/2004	Dycus et al.
6,090,107 A	7/2000	Borgmeier et al.	2004/0122423 A1	6/2004	Dycus et al.
6,096,037 A	8/2000	Mulier et al.	2004/0143263 A1	7/2004	Schechter et al.
6,099,550 A	8/2000	Yoon	2004/0147925 A1	7/2004	Buysse et al.
6,102,909 A	8/2000	Chen et al.	2004/0162557 A1	8/2004	Tetzlaff et al.
6,110,171 A	8/2000	Rydell	2004/0176762 A1	9/2004	Lawes et al.
6,113,596 A	9/2000	Hooven et al.	2004/0225288 A1	11/2004	Buysse et al.
6,113,598 A	9/2000	Baker	2004/0236325 A1	11/2004	Tetzlaff et al.
6,126,658 A	10/2000	Baker	2004/0243125 A1	12/2004	Dycus et al.
6,152,923 A	11/2000	Ryan	2004/0249371 A1	12/2004	Dycus et al.
6,174,309 B1	1/2001	Wrublewski et al.	2004/0249374 A1	12/2004	Tetzlaff et al.
6,179,834 B1	1/2001	Buysse et al.	2004/0250419 A1	12/2004	Sremcich et al.
6,179,837 B1	1/2001	Hooven	2004/0254573 A1	12/2004	Dycus et al.
6,183,467 B1	2/2001	Shapeton et al.	2005/0004568 A1	1/2005	Lawes et al.
6,187,003 B1	2/2001	Buysse et al.	2005/0004570 A1	1/2005	Chapman et al.
6,190,386 B1	2/2001	Rydell	2005/0021025 A1	1/2005	Buysse et al.
6,193,718 B1	2/2001	Kortenbach et al.	2005/0021026 A1	1/2005	Baily
6,206,877 B1	3/2001	Kese et al.	2005/0021027 A1	1/2005	Shields et al.
6,224,593 B1	5/2001	Ryan et al.			
6,228,080 B1	5/2001	Gines			
6,228,083 B1	5/2001	Lands et al.			
6,267,761 B1	7/2001	Ryan			
6,270,508 B1	8/2001	Klieman et al.			
6,273,887 B1	8/2001	Yamauchi et al.			

FOREIGN PATENT DOCUMENTS

EP	0364216 A1	4/1990
EP	0518230 A1	12/1992
EP	0 541 930 B1	5/1993

EP	0572131		12/1993	Heniford et al. "Initial Results with an Electrothermal Bipolar Vessel Sealer" <i>Surgical Endoscopy</i> (2000) 15:799-801.
EP	0584787	A1	3/1994	Crawford et al. "Use of the LigaSure Vessel Sealing System in Urologic Cancer Surgery" <i>Grand Rounds In Urology</i> 1999 vol. 1 issue 4 pp. 10-17.
EP	0623316	A1	11/1994	Rothenberg et al. "Use of the LigaSure Vessel Sealing System in Minimally Invasive Surgery in Children" <i>INT'L Pediatric Endosurgery Group (IPEG)</i> 2000.
EP	0624348	A2	11/1994	Palazzo et al. "Randomized clinical trial of LigaSure versus open haemorrhoidectomy" <i>British Journal Of Surgery</i> 2002, 89, 154-157.
EP	EP 0624348	A2	11/1994	"Innovations in Electrosurgery" Sales/Product Literature.
EP	0650701	A1	5/1995	LigaSure Vessel Sealing System, the Seal of Confidence in General, Gynecologic, Urologic, and Laparoscopic Surgery Sales/Product Literature.
EP	0694290	A3	3/1996	Carbonell et al., "Comparison of theGyrus PlasmaKinetic Sealer and the Valleylab LigaSure Device in the Hemostasis of Small, Medium, and Large-Sized Arteries".
EP	0717966	A1	6/1996	"Reducing Needlestick Injuries in the Operating Room" Sales/Product Literature.
EP	0754437	A3	3/1997	Chung et al., "Clinical Experience of Sutureless Closed Hemorrhoidectomy with LigaSure" <i>Diseases of the Colon & Rectum</i> vol. 46. No. 1 Jan. 2003.
EP	0853922	A1	7/1998	Strasberg et al., "Use of a Bipolar Vessel-Sealing Device for Parenchymal Transection During Liver Surgery" <i>Journal of Gastrointestinal Surgery</i> , vol. 6, No. 4, Jul./Aug. 2002 pp.569-574.
EP	0887046	A3	1/1999	Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" <i>The American Journal of Suregry</i> , vol. 181, No. 3, □Apr. 2001 pp. 236-237.
EP	0923907	A1	6/1999	W. Scott Helton, "LigaSure Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery" Sales/Product Literature.
EP	1034747	A1	9/2000	Michael Choti, "Abdominoperinal Resection with the LigaSure Vessel Sealing System and LigaSure Atlas 20 cm Open Instrument" <i>Innovations That Work</i> , □Jun. 2003.
EP	1034748	A1	9/2000	Craig Johnson, "Use of the LigaSure Vessel Sealing System in Bloodless Hemorrhoidectomy" <i>Innovations That Work</i> , □Mar. 2000.
EP	1025807	A3	10/2000	Muller et al., "Extended Left Hemicolectomy Using the LigaSure Vessel Sealing System" <i>Innovations That Work</i> , □Sep. 1999.
EP	1034746	A3	10/2000	Herman et al., "Laparoscopic Intestinal Resection With the LigaSure Vessel Sealing System: A Case Report" <i>Innovations That Work</i> , □Feb. 2002.
EP	1050278	A1	11/2000	Carus et al., "Initial Experience With The LigaSure Vessel Sealing System in Abdominal Surgery" <i>Innovations That Work</i> , □Jun. 2002.
EP	1053719	A1	11/2000	Levy et al., "Randomized Trial of Suture Versus Electrosurgical Bipolar Vessel Sealing in Vaginal Hysterectomy" <i>Obstetrics & Gynecology</i> , vol. 102, No. 1, Jul. 2003.
EP	1053720	A1	11/2000	Levy et al., "Update on Hysterectomy— New Technologies and Techniques" <i>OBG Management</i> , Feb. 2003.
EP	1055399	A1	11/2000	Barbara Levy, "Use of a New Vessel Ligation Device During Vaginal Hysterectomy" <i>FIGO</i> 2000, Washington, D.C.
EP	1055400	A1	11/2000	McLellan et al. "Vessel Sealing for Hemostasis During Gynecologic Surgery" Sales/Product Literature.
EP	1080694	A1	3/2001	Sengupta et al., "Use of a Computer-Controlled Bipolar Diathermy System in Radical Prostatectomies and Other Open Urological Surgery" <i>ANZ Journal of Surgery</i> (2001) 71.9 pp. 538-540.
EP	1082944	A1	3/2001	Olsson et al. "Radical Cystectomy in Females" <i>Current Surgical Techniques in Urology</i> , vol. 14, Issue 3.
EP	1159926	A2	12/2001	E. David Crawford "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Veinous Complex" Sales/Product Literature.
EP	EP 1159926	A2	12/2001	Jarrett et al., "Use of the LigaSure Vessel Sealing System for Per-Hilar Vessels in Laparoscopic Nephrectomy" Sales/Product Literature.
GB	2214430	A	6/1989	E. David Crawford "Evaluation of a New Vessel Sealing Device in Urologic Cancer Surgery" Sales/Product Literature.
WO	WO 92/06842		4/1992	Joseph Ortenberg "LigaSure System Used in Laparoscopic 1st and 2nd Stage Orchiopexy" <i>Innovations That Work</i> , Nov. 2002.
WO	WO 94/08524	A	4/1994	Koyle et al., "Laparoscopic Palomo Varicocele Ligation in Children and Adolescents" <i>Pediatric Endosurgery & Innovative Techniques</i> , vol. 6, No. 1, 2002.
WO	WO 95/02369		1/1995	
WO	WO 96/13218		9/1996	
WO	WO 97/00646		1/1997	
WO	WO 97/00647		1/1997	
WO	WO 97/24073		7/1997	
WO	WO 97/24993		7/1997	
WO	WO 98/27880		7/1998	
WO	WO 99/03407		1/1999	
WO	WO 99/03408		1/1999	
WO	WO 99/03409		1/1999	
WO	WO99/12488		3/1999	
WO	WO 99/12488	A	3/1999	
WO	WO 99/40857		8/1999	
WO	WO 99/51158		10/1999	
WO	WO 99/66850	A	12/1999	
WO	WO 00/24330		5/2000	
WO	WO 00/41638		7/2000	
WO	WO 00/53112		9/2000	
WO	WO 01/17448	A	3/2001	
WO	WO 01/54604		8/2001	
WO	WO 02/080795		10/2002	
WO	WO 02/080796	A1	10/2002	
WO	WO 02/080798		10/2002	
WO	WO 02/080798	A1	10/2002	
WO	WO 02/080799		10/2002	
WO	WO 2004/052221	A1	6/2004	
WO	WO 2004/082495	A1	9/2004	
WO	WO 2004/098383	A1	11/2004	

OTHER PUBLICATIONS

- Bergdahl et al. "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator" *J. Neurosurg*, vol. 75, Jul. 1991, pp. 148-151.
- Kennedy et al. "High-burst-strength, feedback-controlled bipolar vessel sealing" *Surgical Endoscopy* (1998) 12: 876-878.
- Peterson et al. "Comparison of Healing Process Following Ligation with Sutures and Bipolar Vessel Sealing" *Surgical Technology International* (2001).
- Linehan et al. "A Phase I Study of the LigaSure Vessel Sealing System in Hepatic Surgery" Section of HPB Surger, Washington University School of Medicine, St. Louis MO, Presented at AHPBA, Feb. 2001.
- Sayfan et al. "Sutureless Closed Hemorrhoidectomy: A New Technique" *Annals Of Surgery* vol.234 No. 1 Jul. 2001.

Dulemba et al. "Use of a Bipolar Electrothermal Vessel Sealer in Laparoscopically Assisted Vaginal Hysterectomy" Sales/Product Literature.

Johnson et al. "Evaluation of a Bipolar electrothermal Vessel Sealing Device in Hemorrhoidectomy" Sales/Product Literature.

Int'l Search Report PCT/US01/11218.

Int'l Search Report PCT/US99/24869.

Int'l Search Report PCT/US98/18640.

Int'l Search Report PCT/US98/23950.

Int'l Search Report PCT/US04/13273.

Int'l Search Report PCT/US04/15311.

Int'l Search Report PCT/US01/11420.

Int'l Search Report PCT/US02/11100.

PCT/US01/11340 International Search Report.

PCT/US01/11420 International Search Report.

PCT/US0201890 International Search Report.

PCT/US02/11100 International Search Report.

PCT/US04/03436 International Search Report.

PCT/US/04/13273 International Search Report.

PCT/US04/15311 International Search Report.

EP 98944778 International Search Report.

EP 98958575 International Search Report.

EP 04027479 International Search Report.

EP 04027705 International Search Report.

EP 04027314 International Search Report.

* cited by examiner

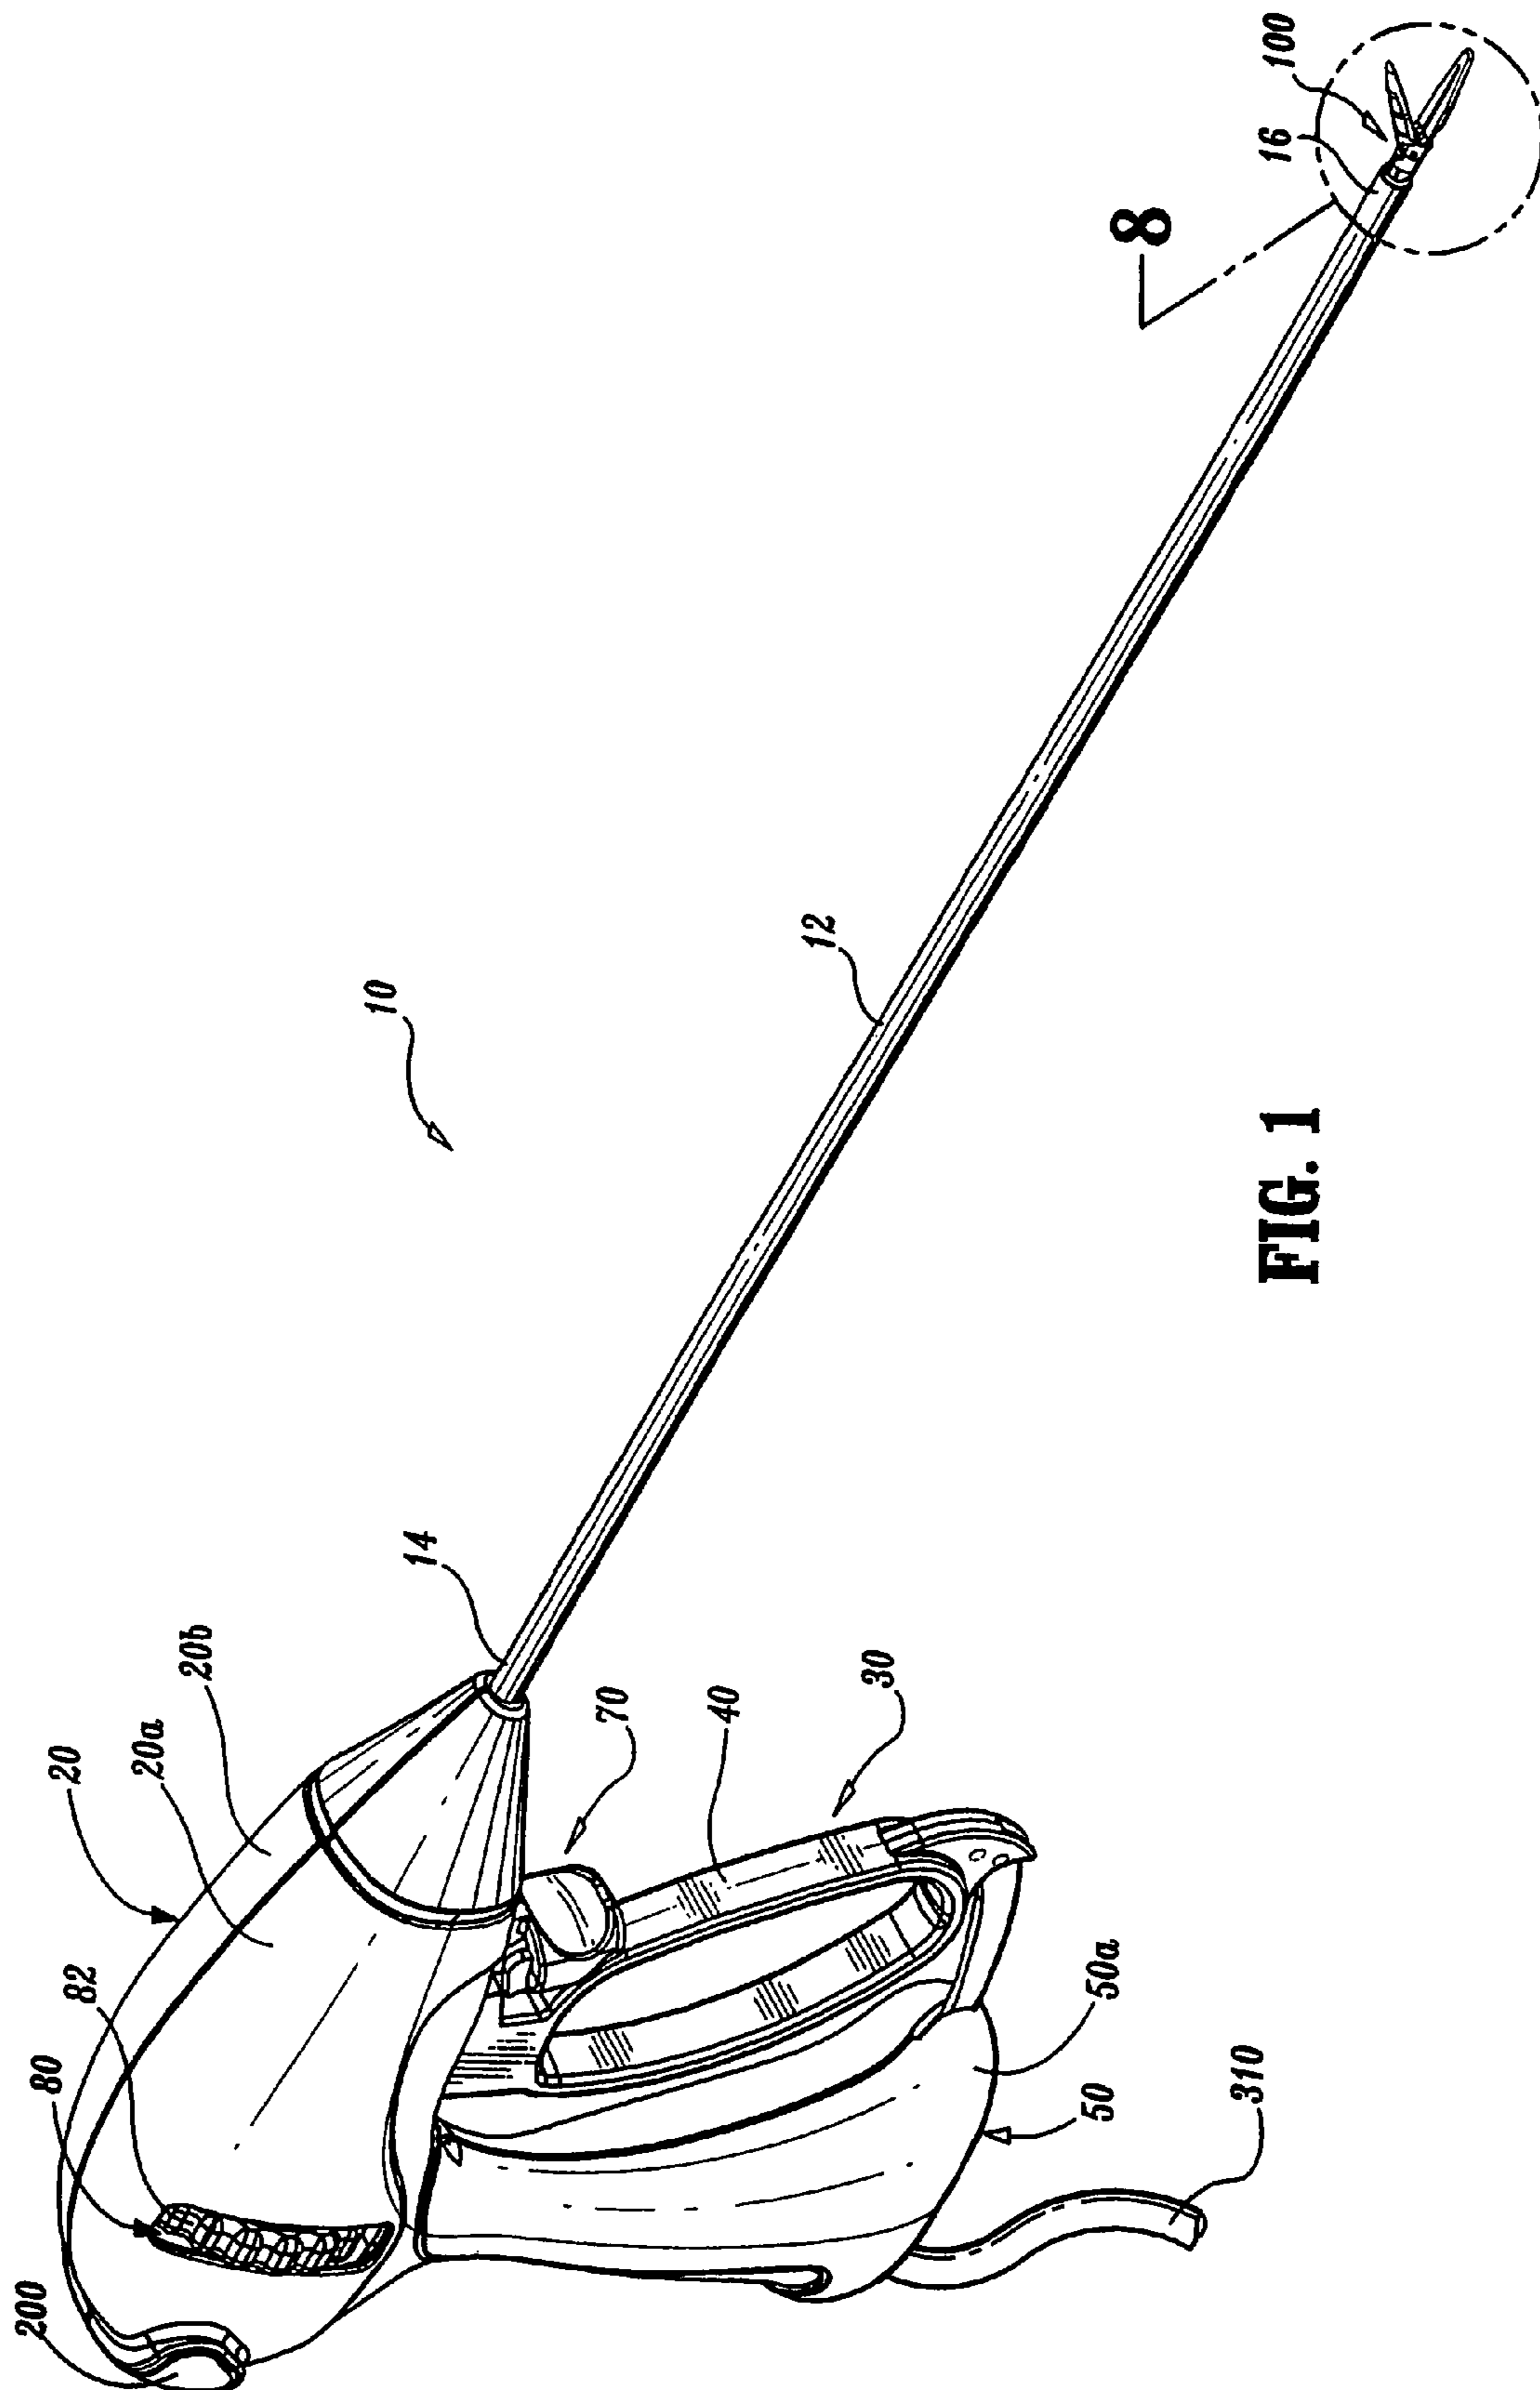


FIG. 1

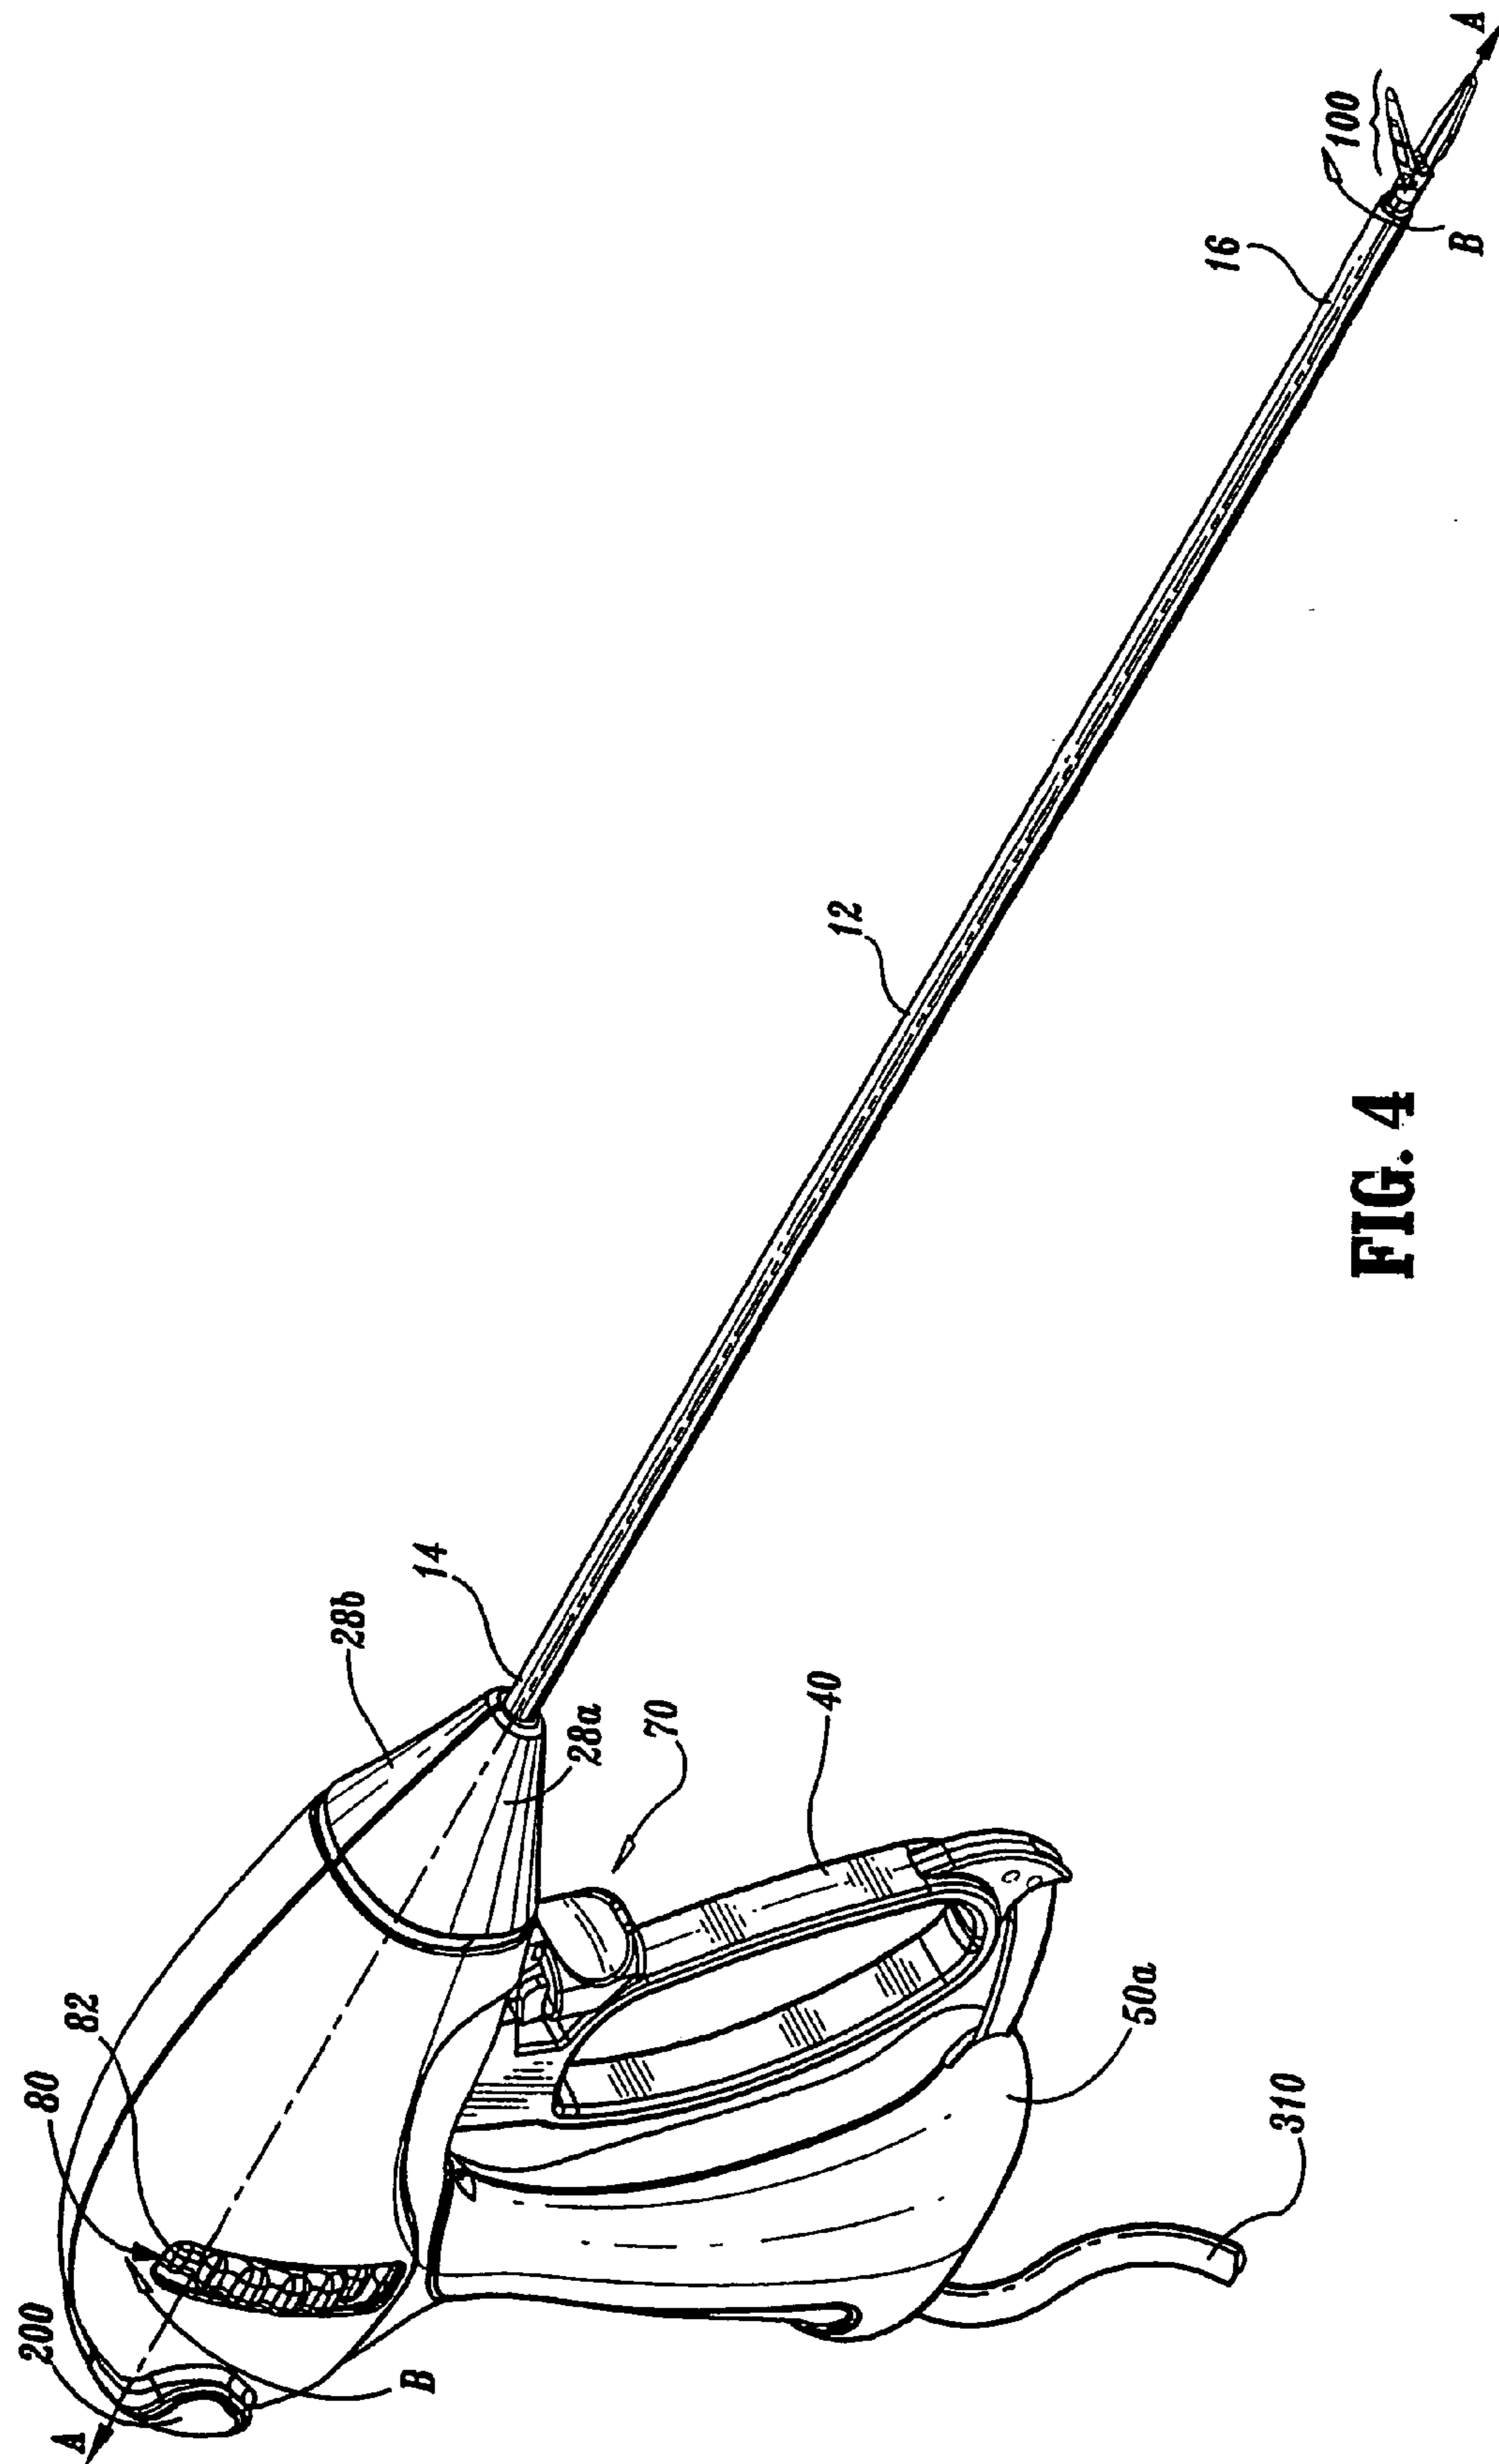


FIG. 4

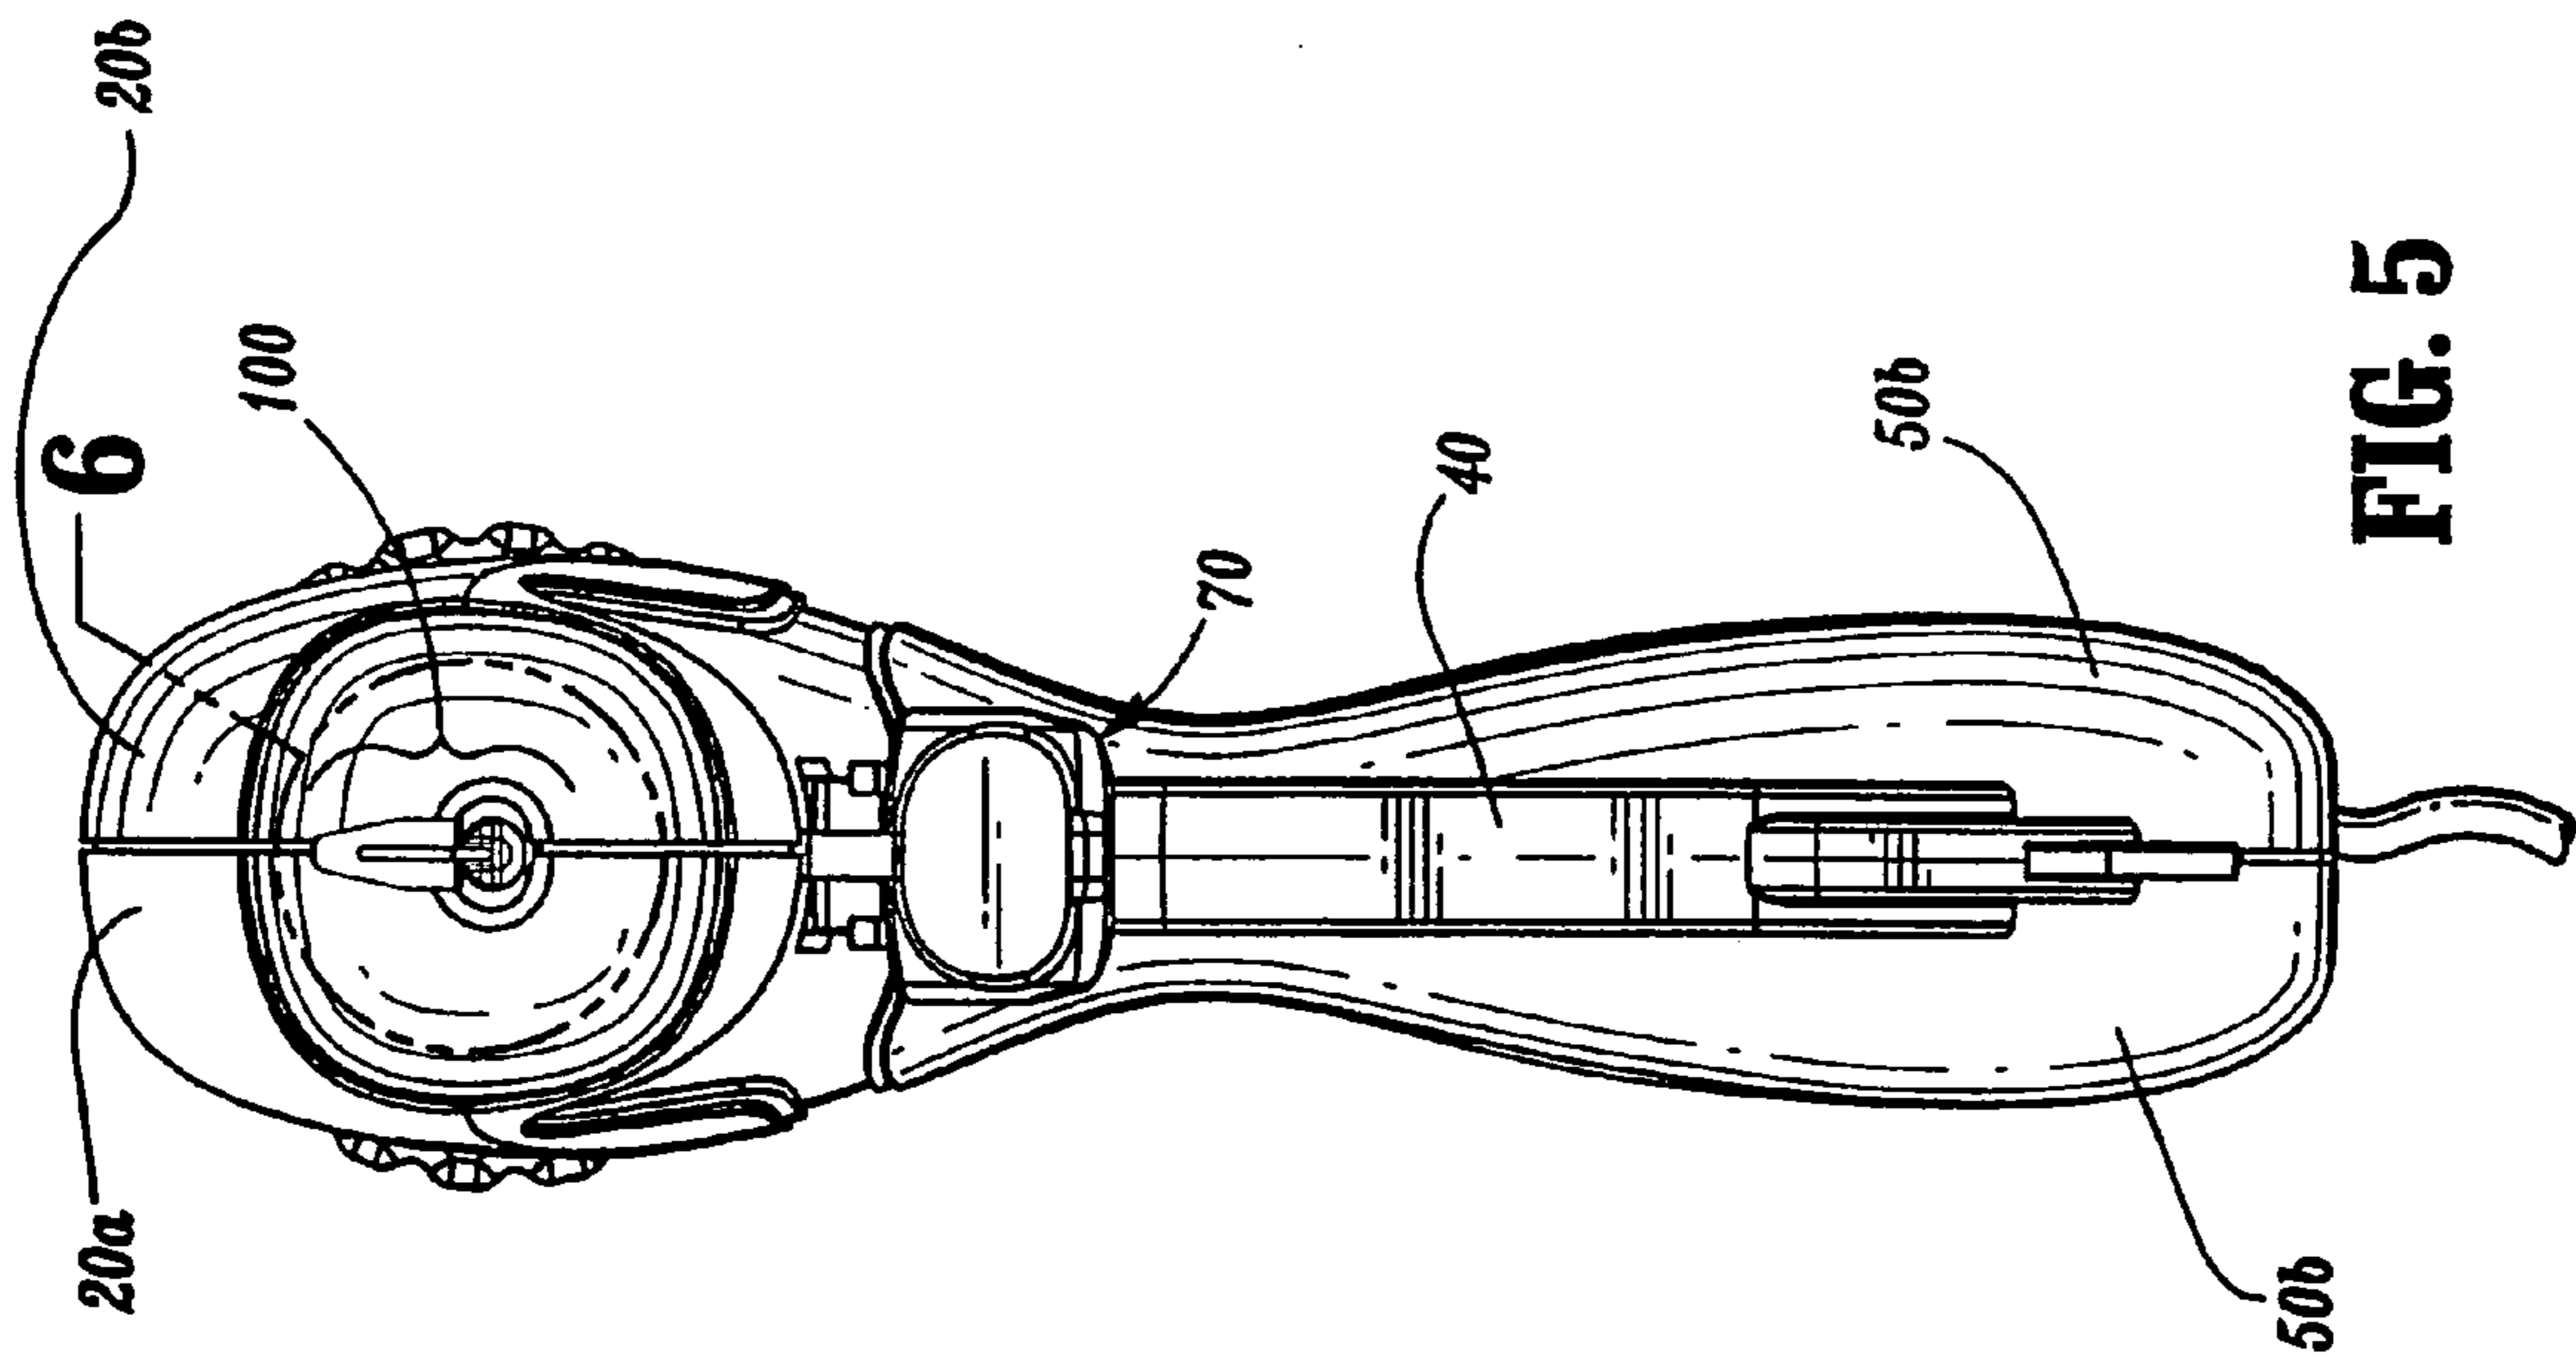


FIG. 5

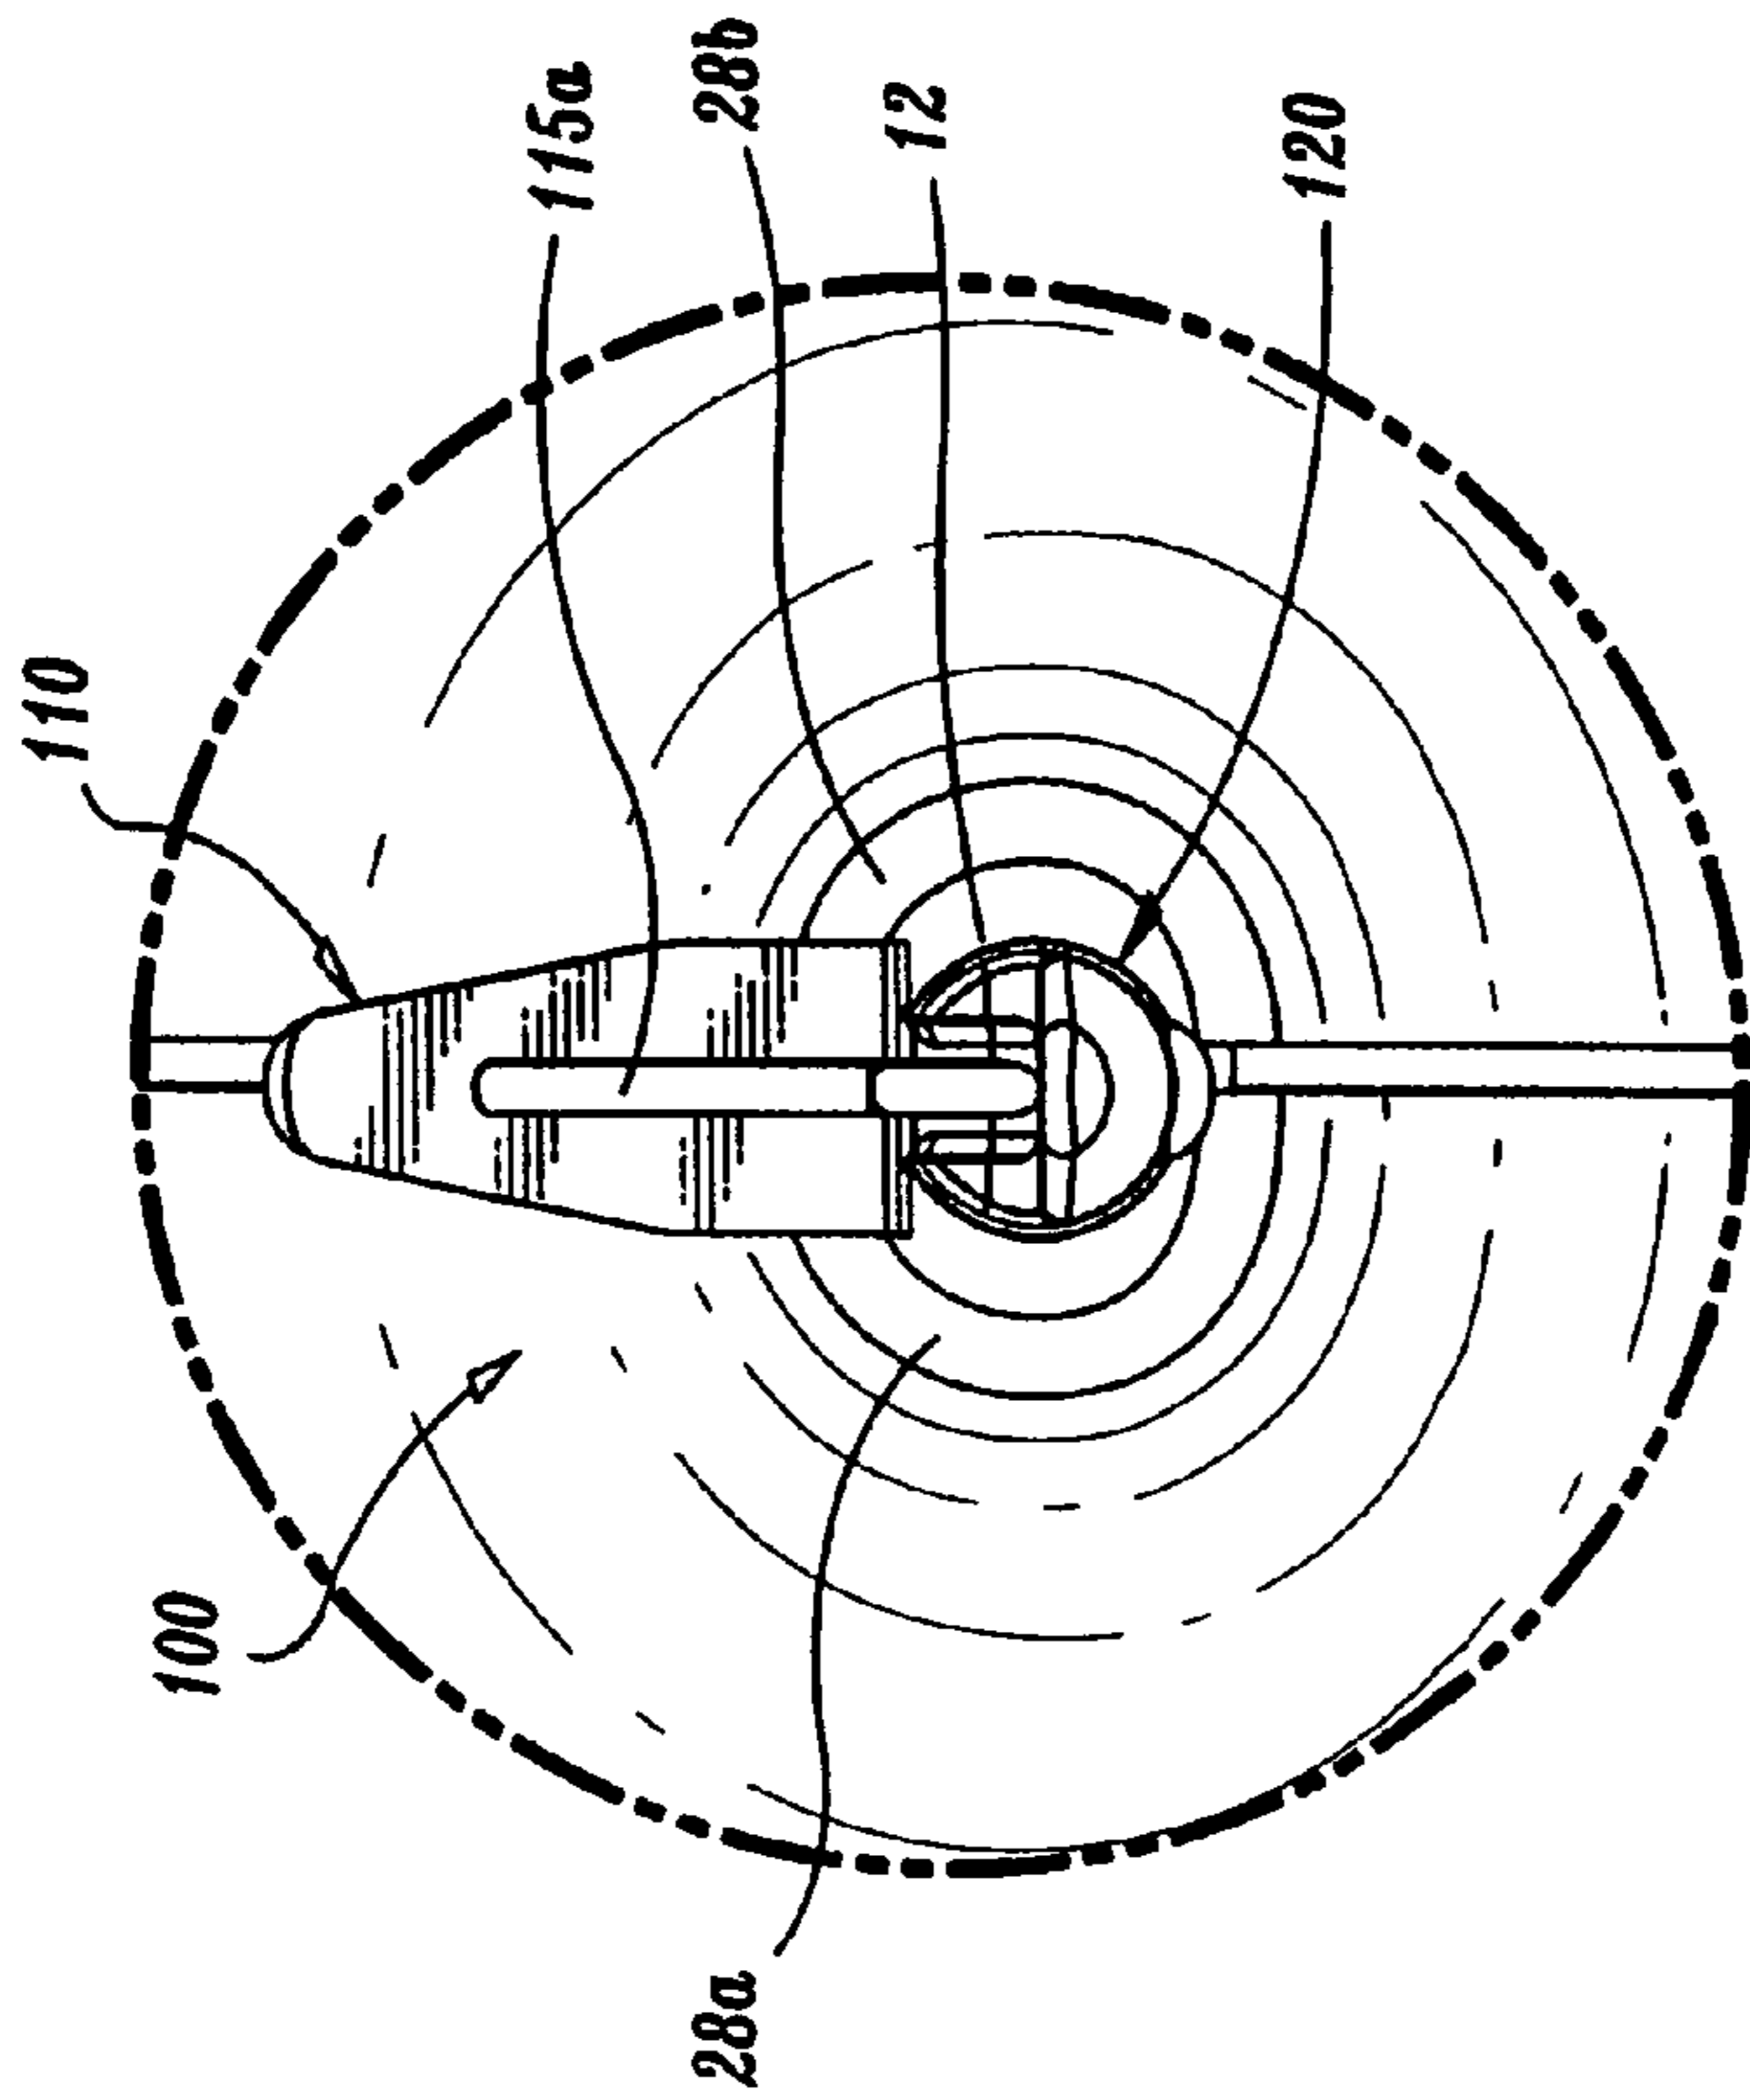


FIG. 6

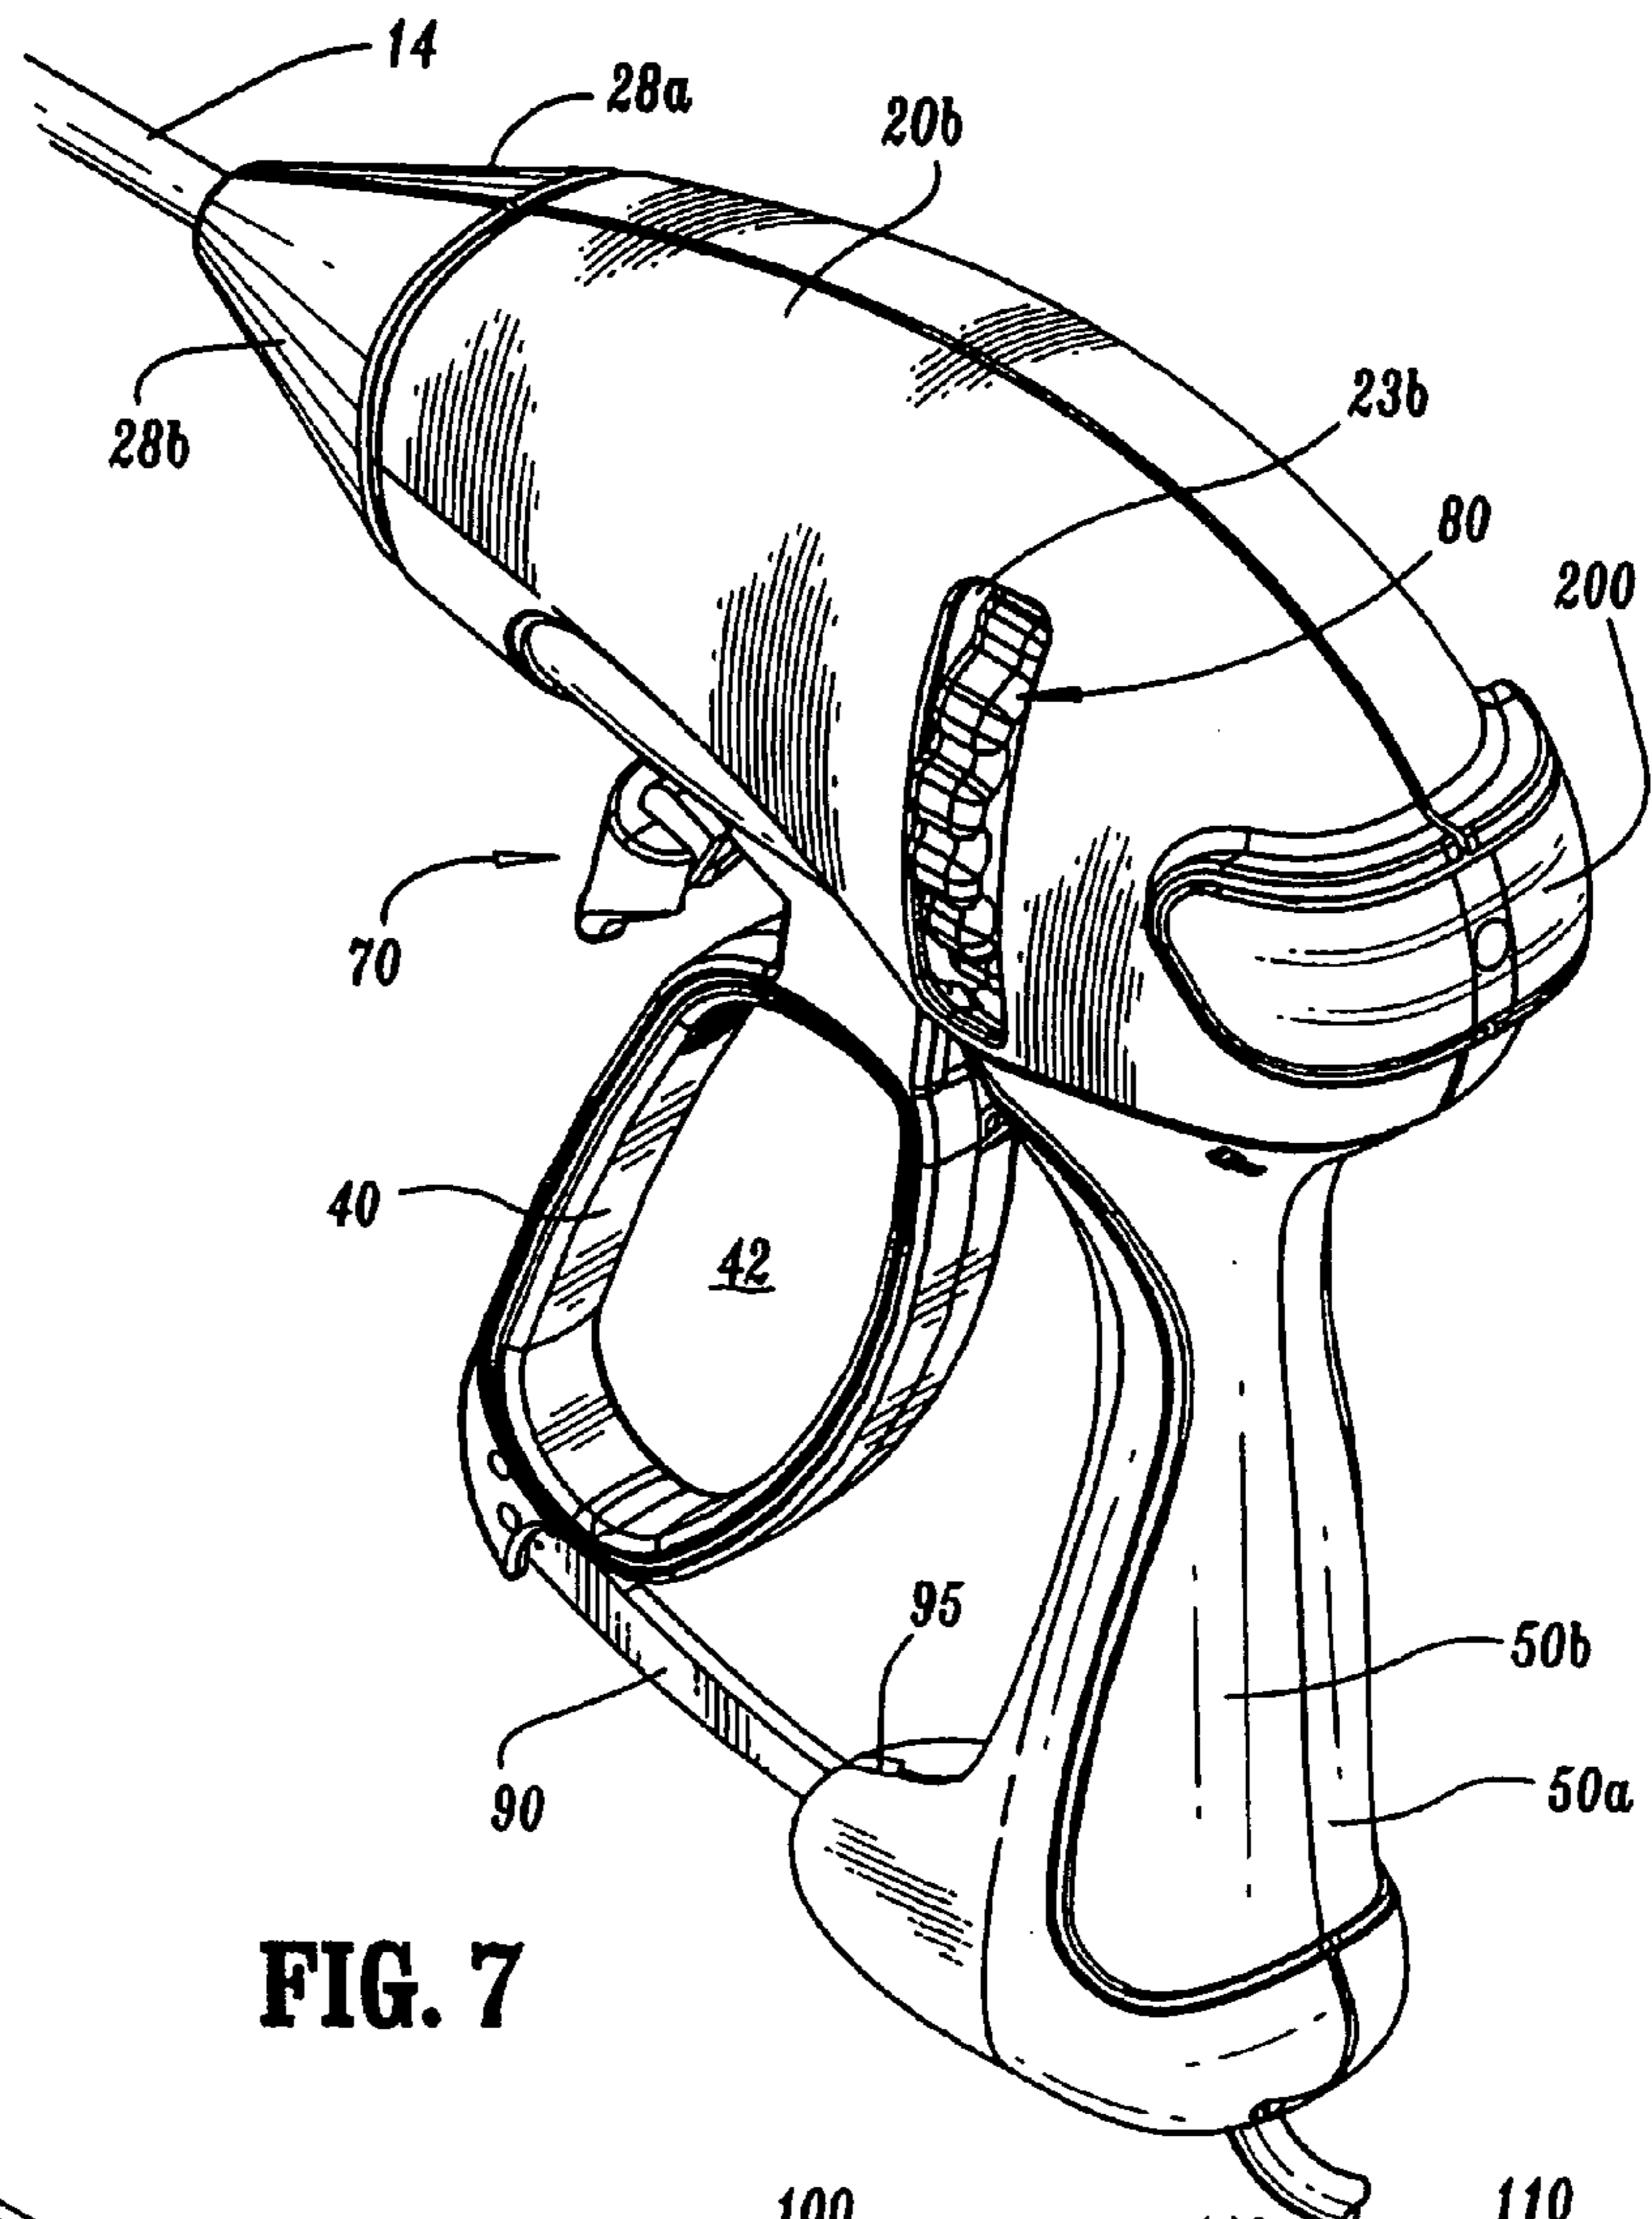


FIG. 7

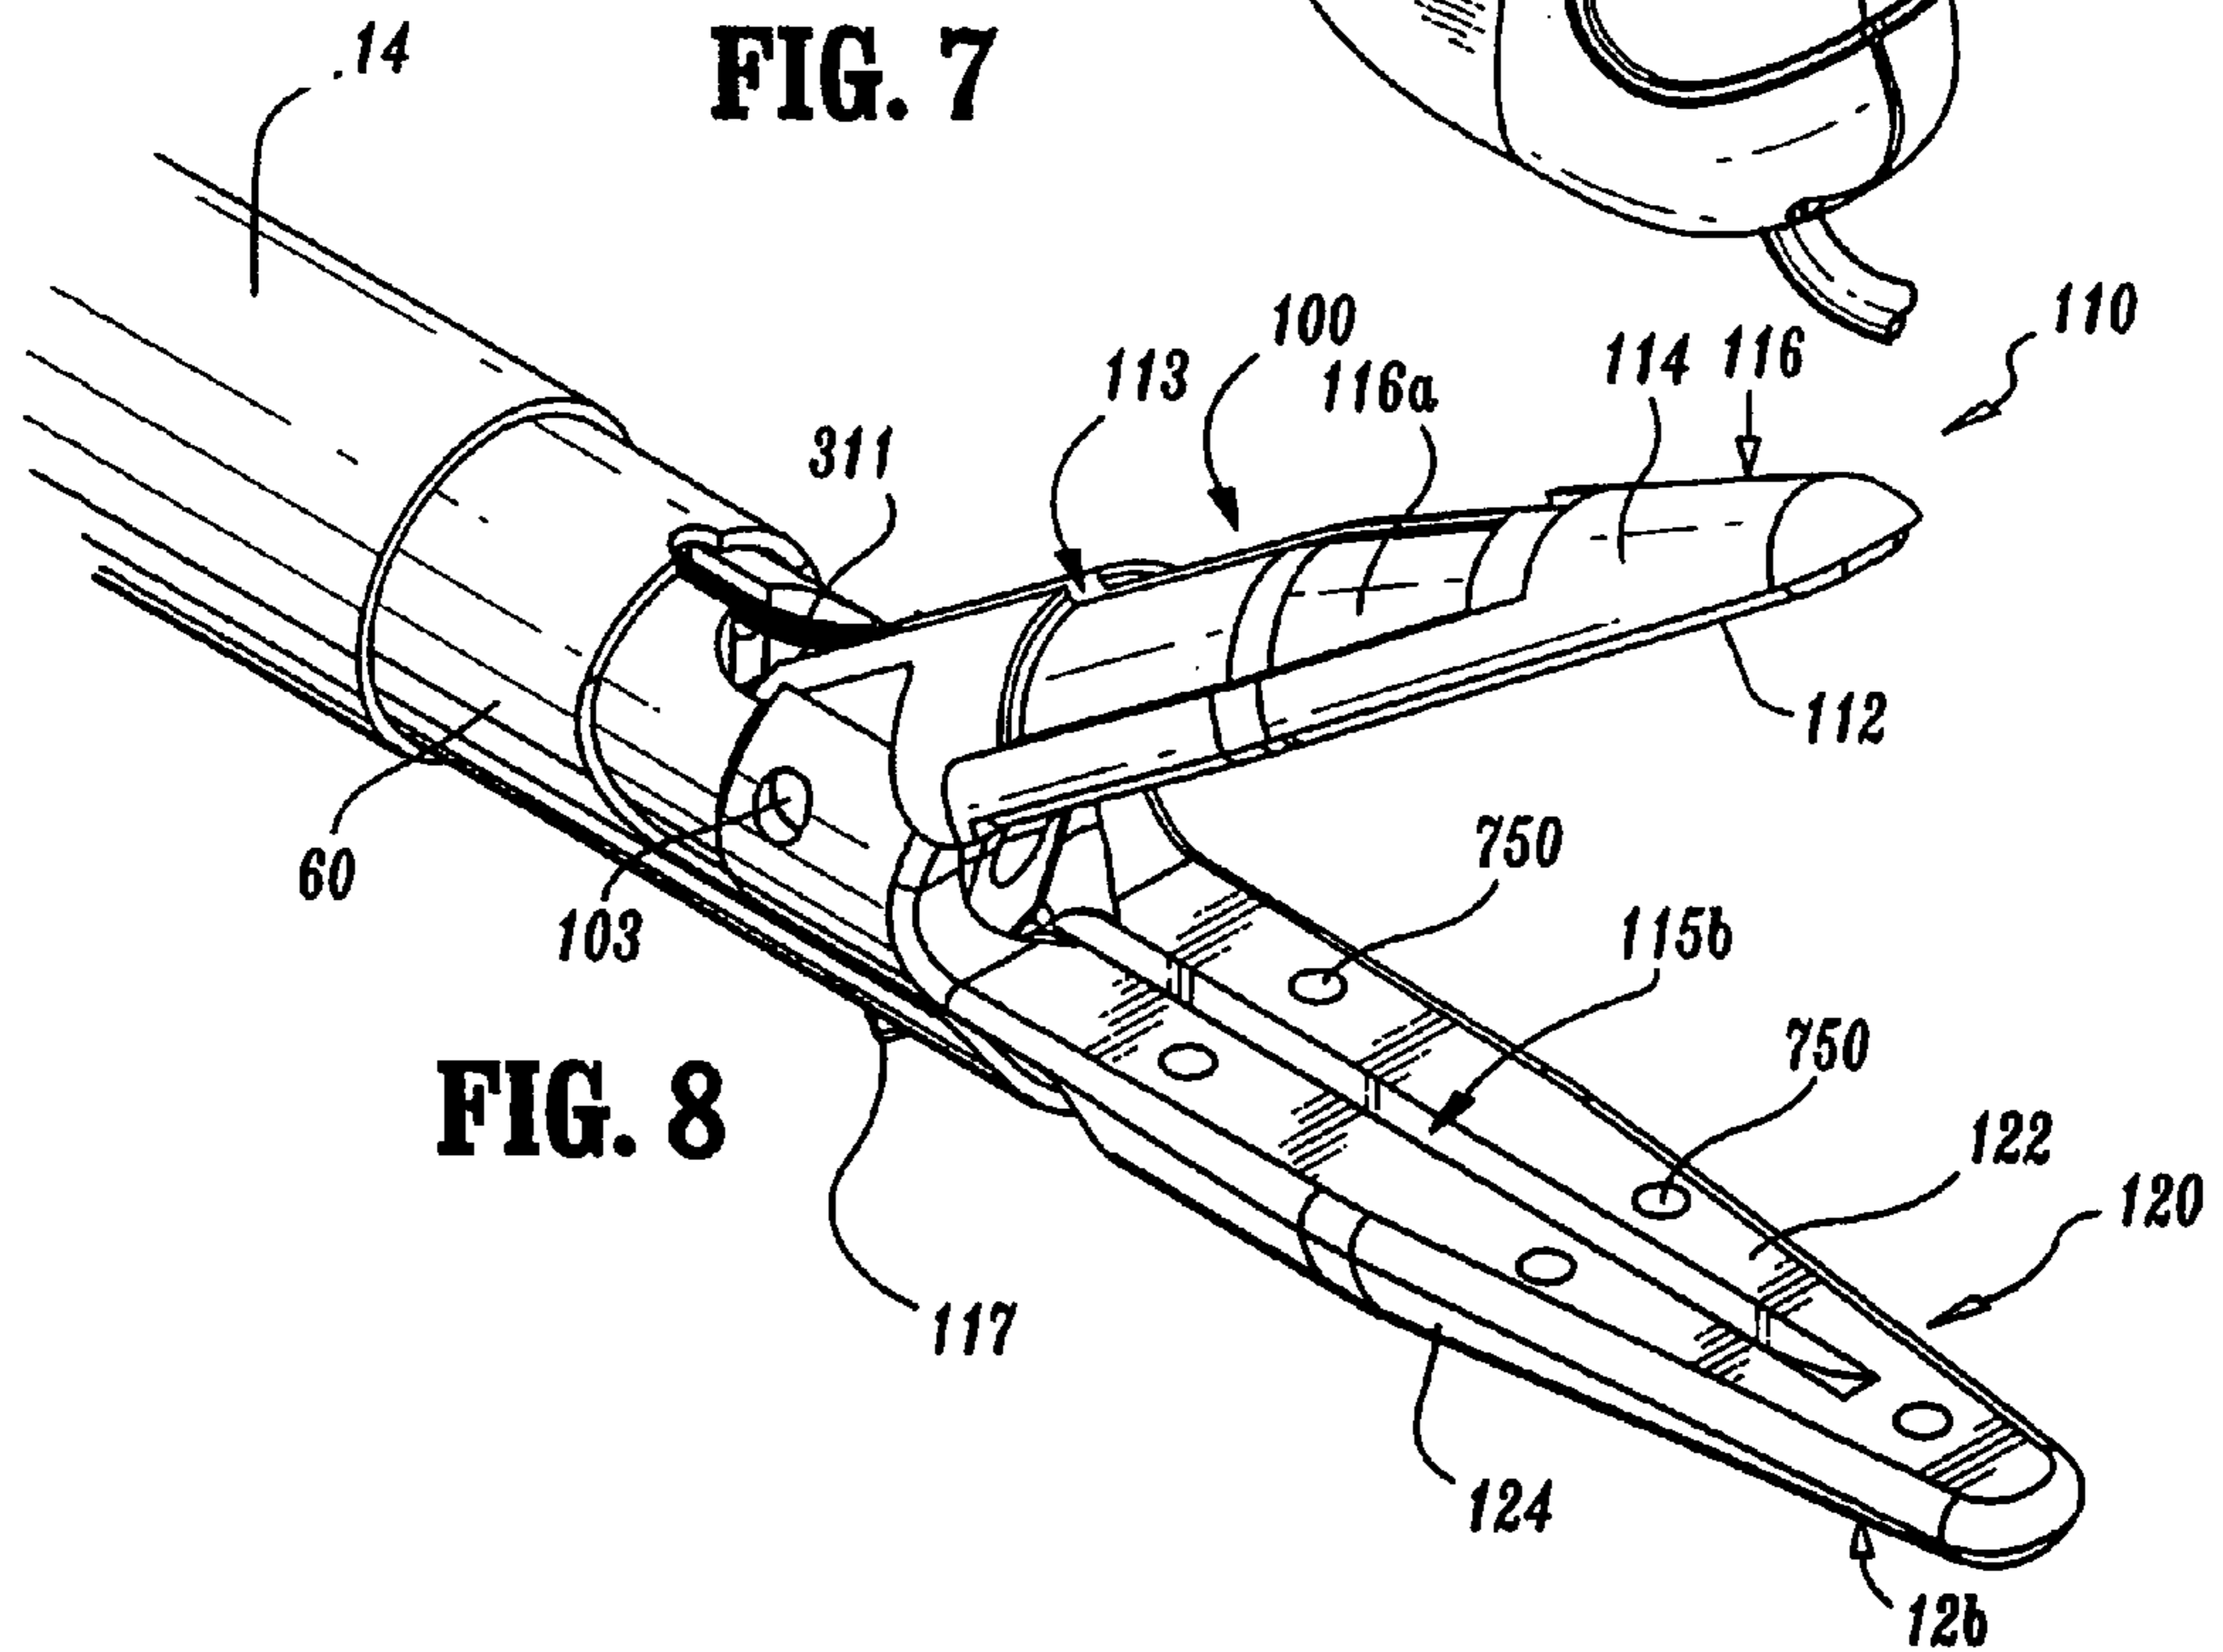


FIG. 8

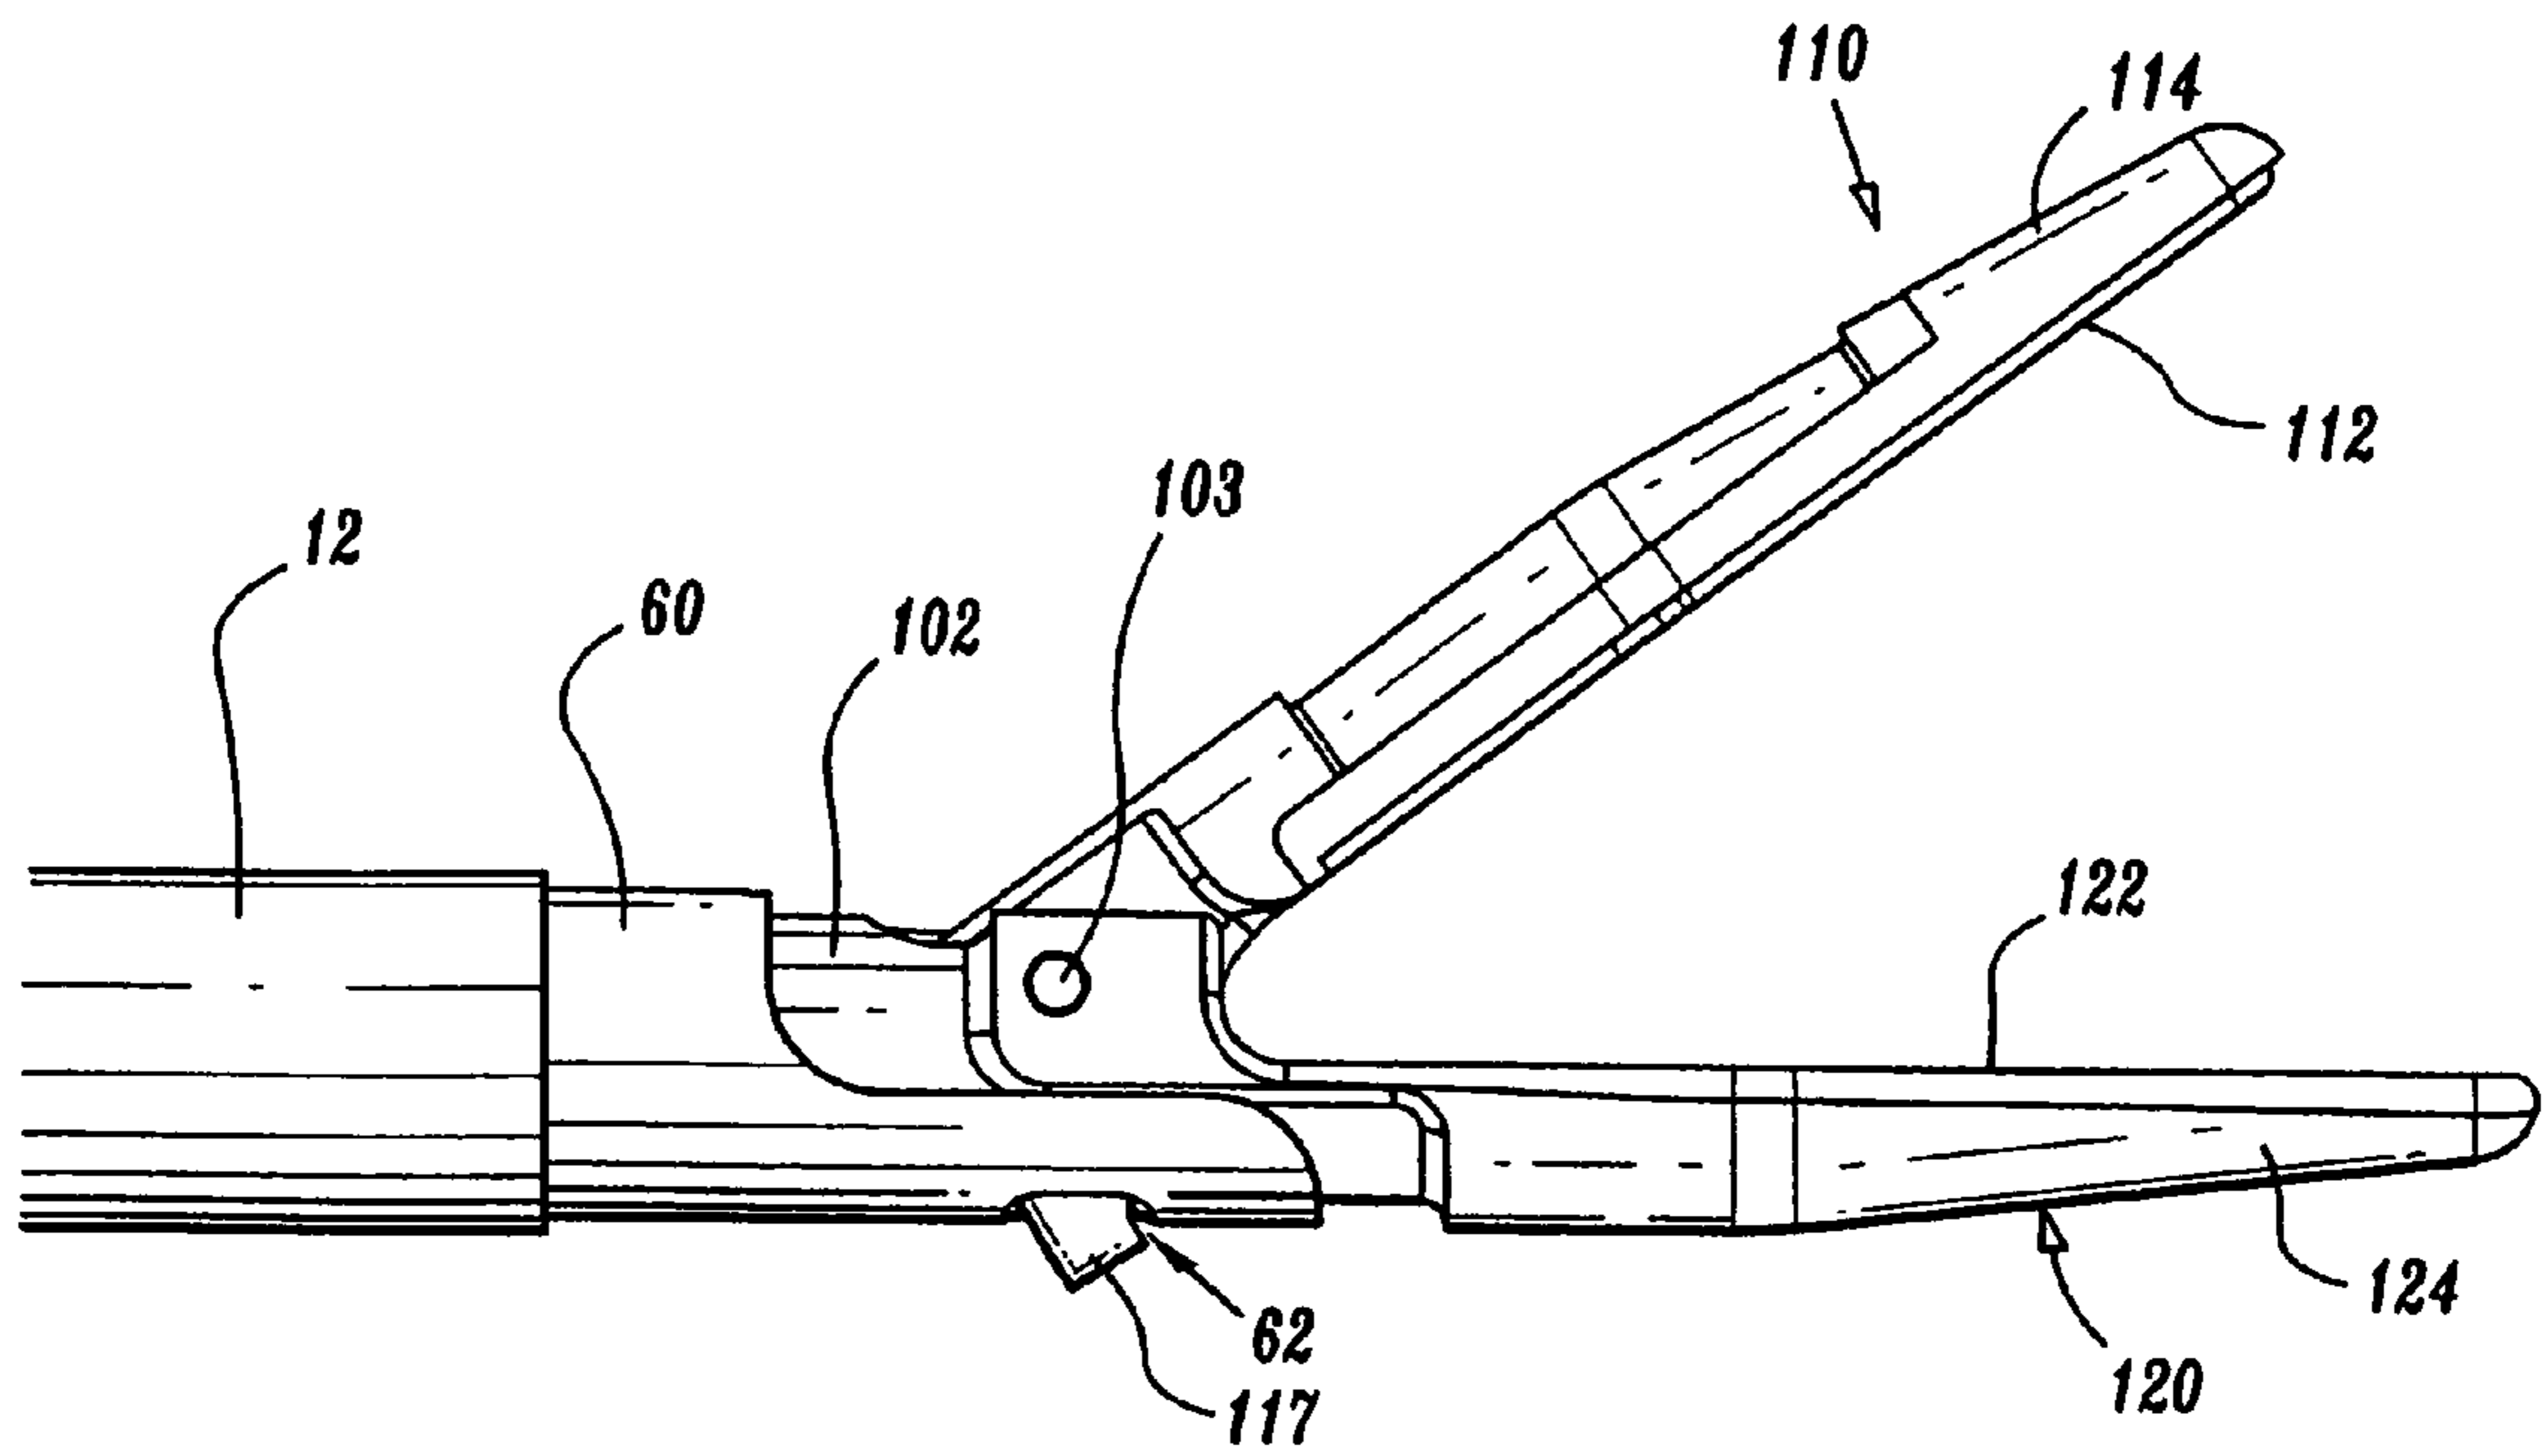


FIG. 9

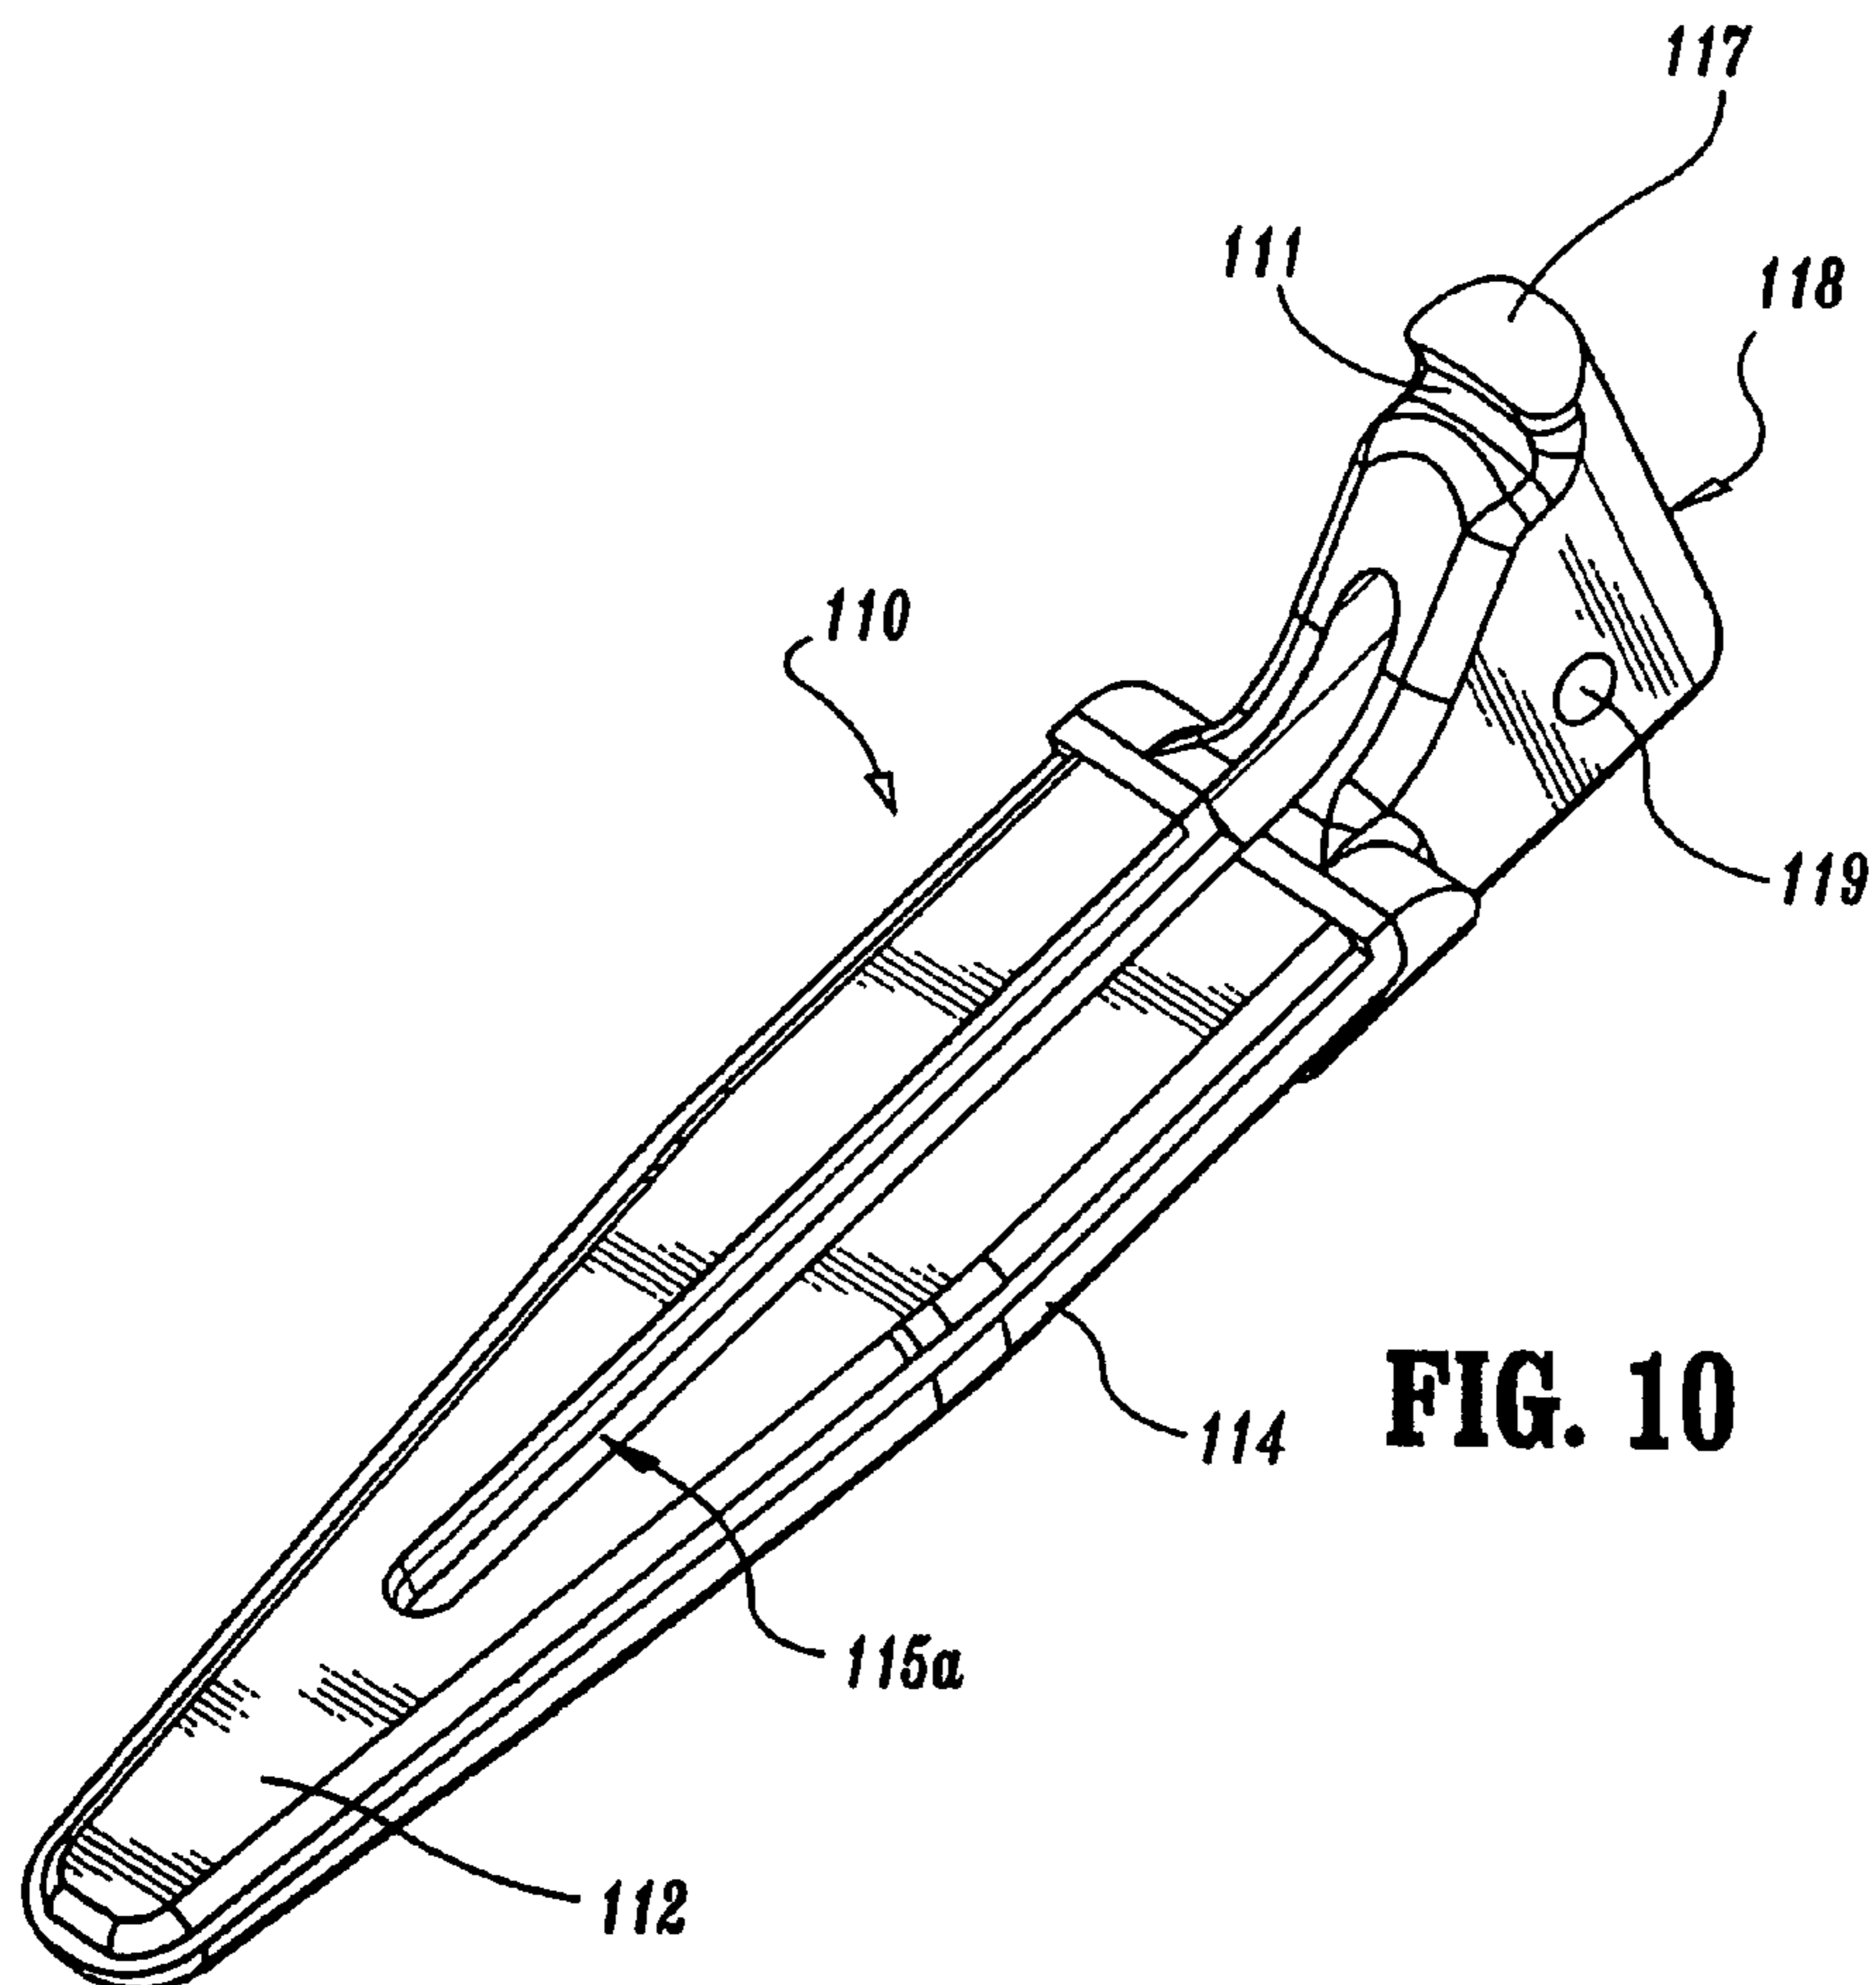


FIG. 10

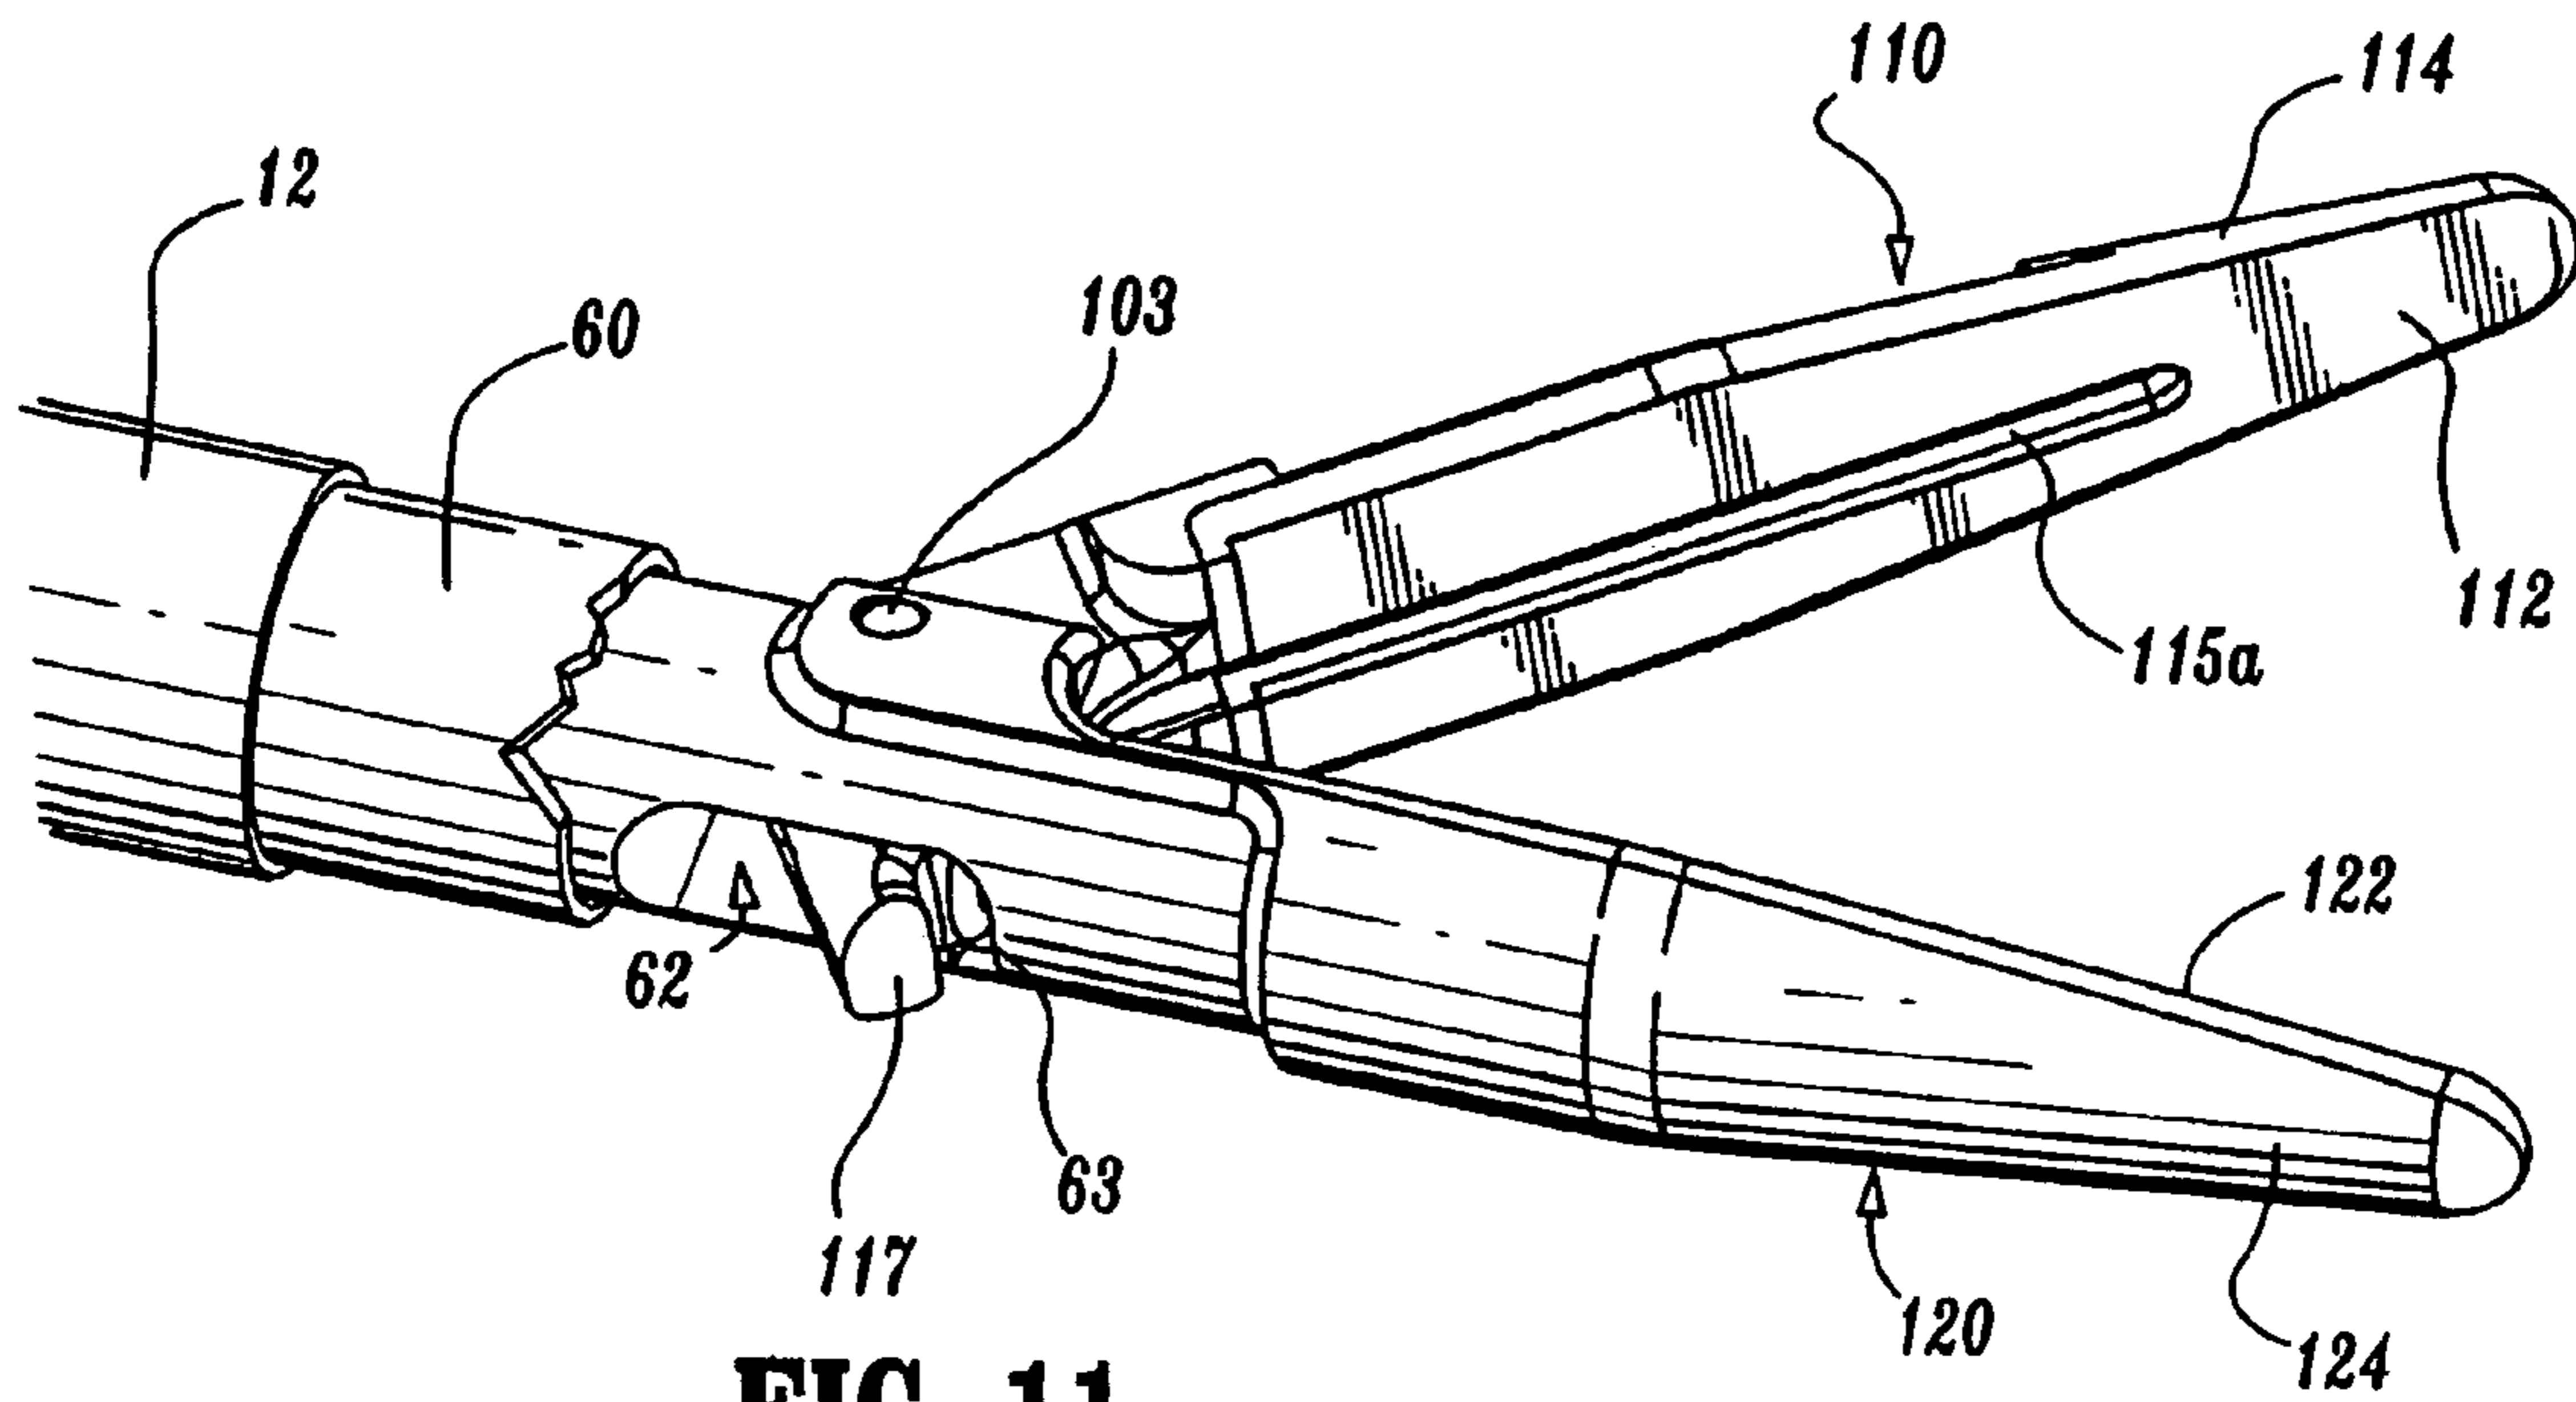


FIG. 11

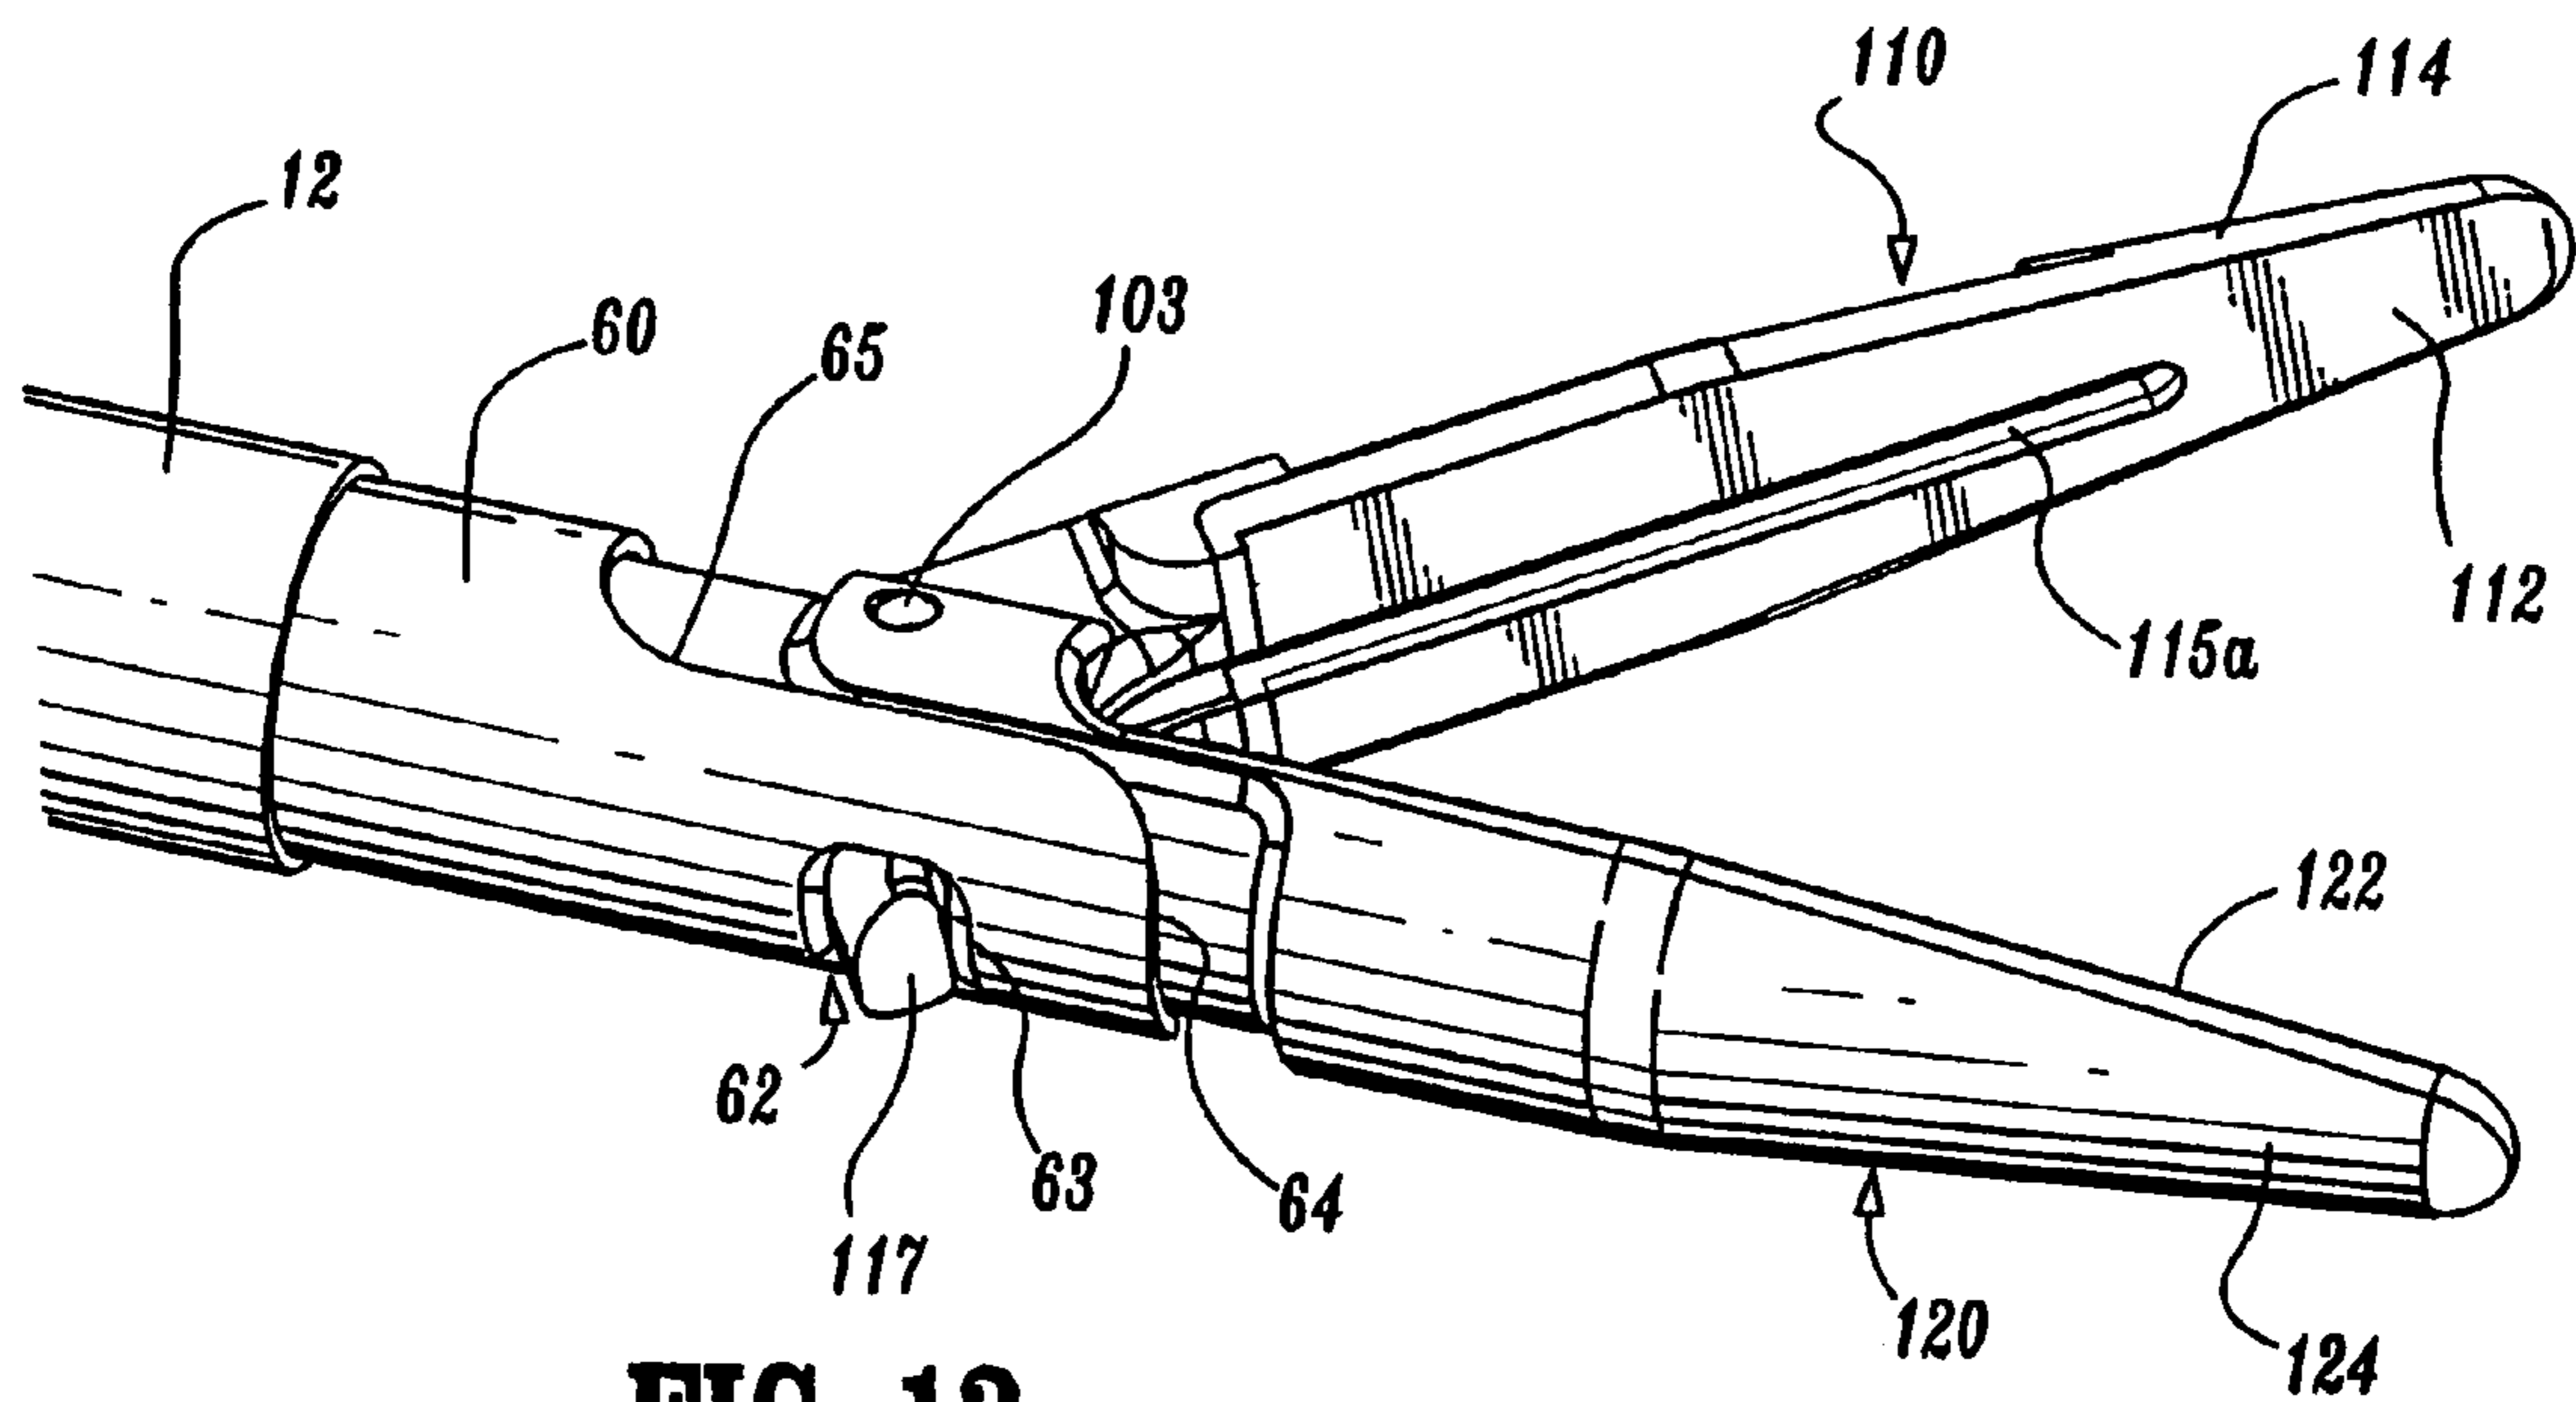


FIG. 12

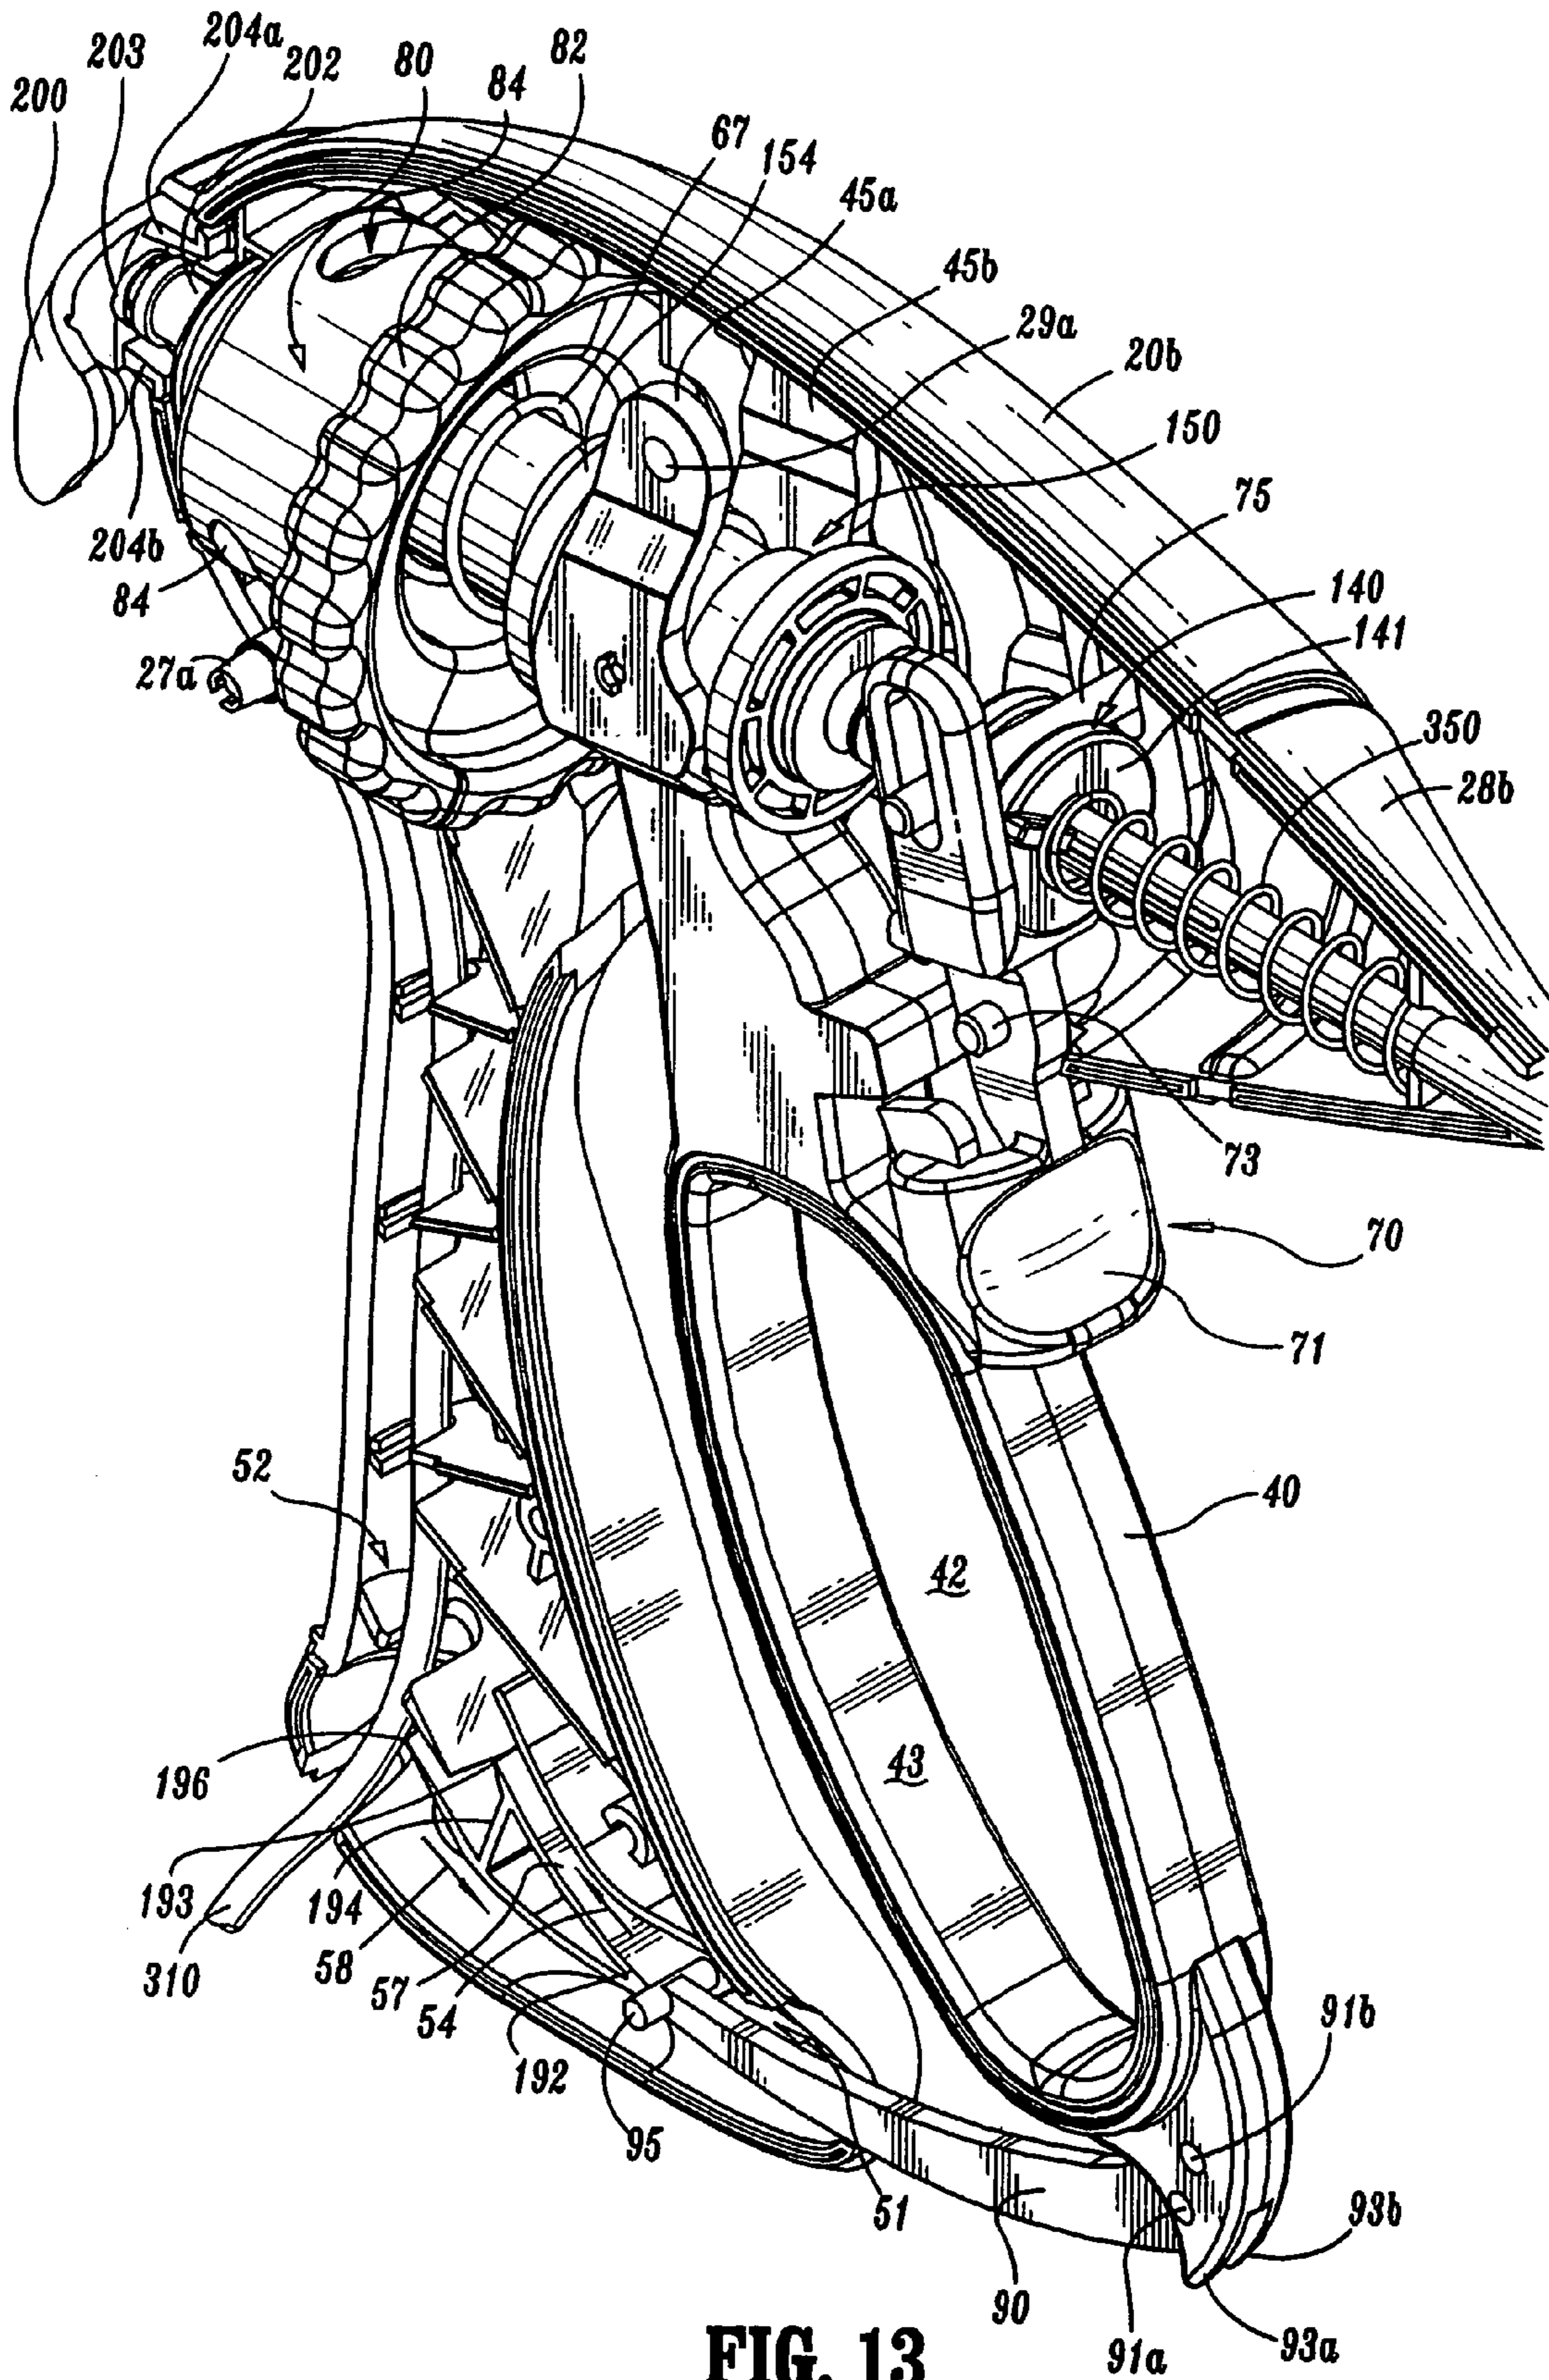
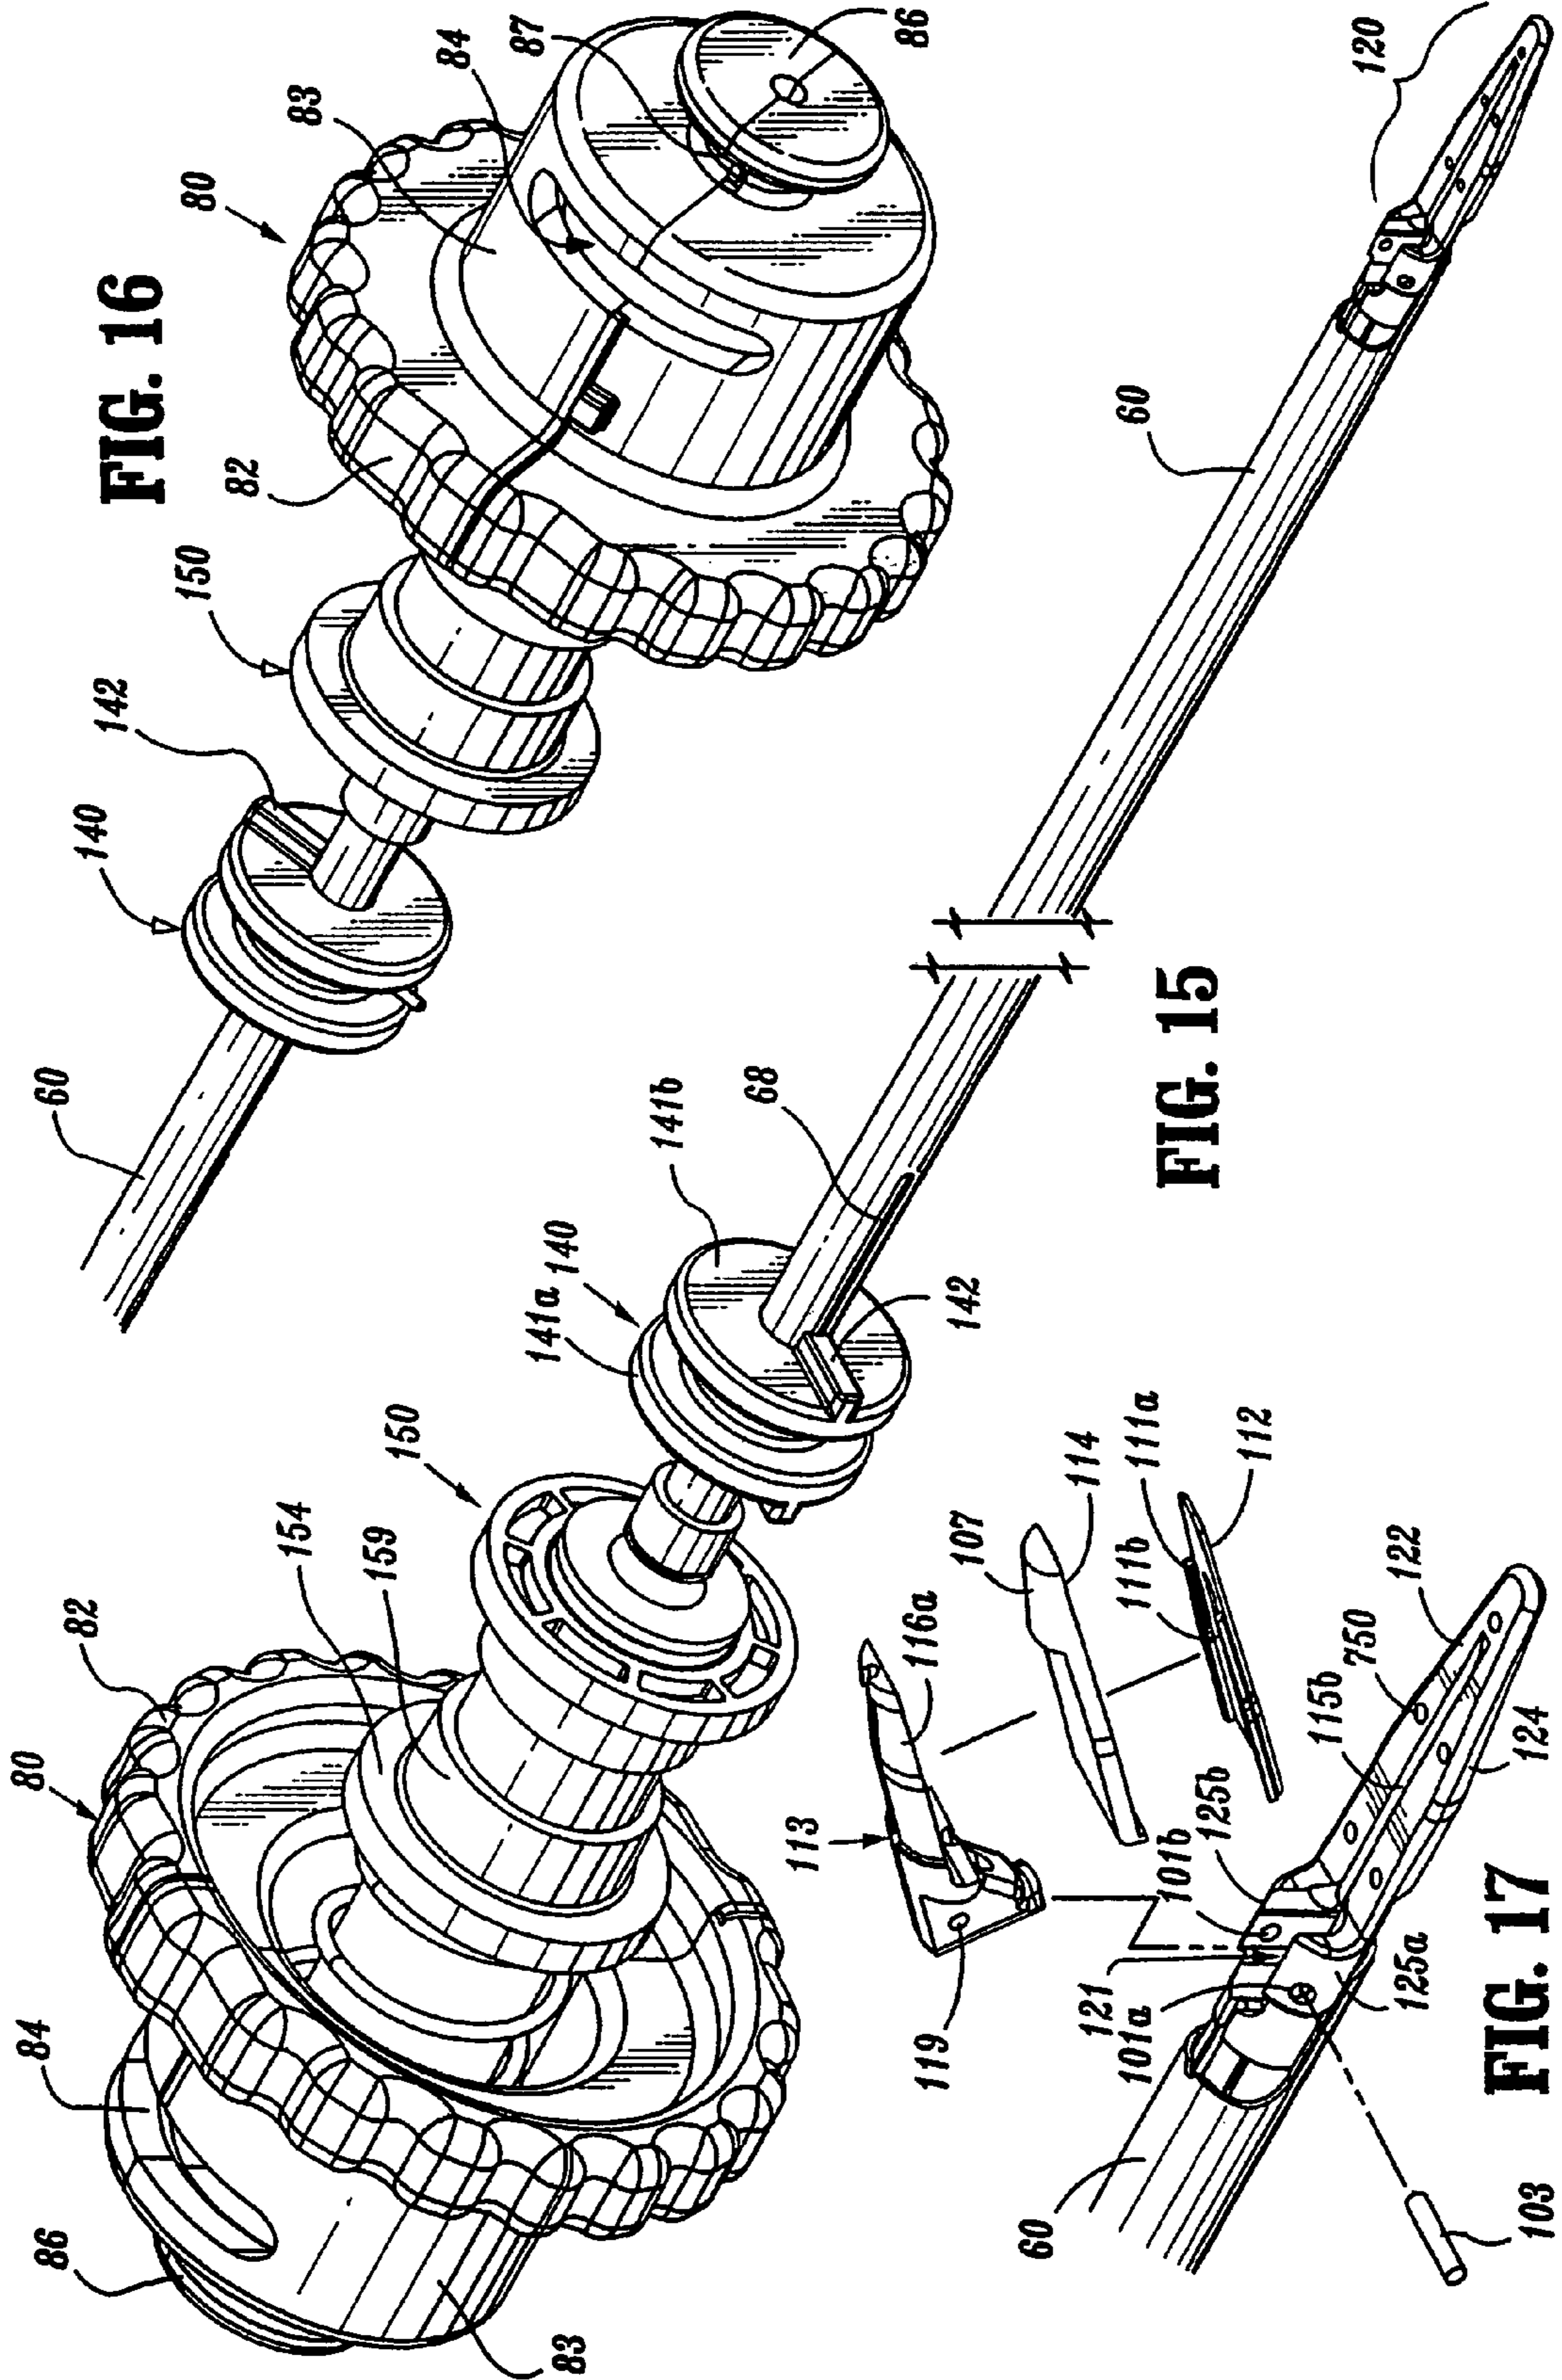


FIG. 13



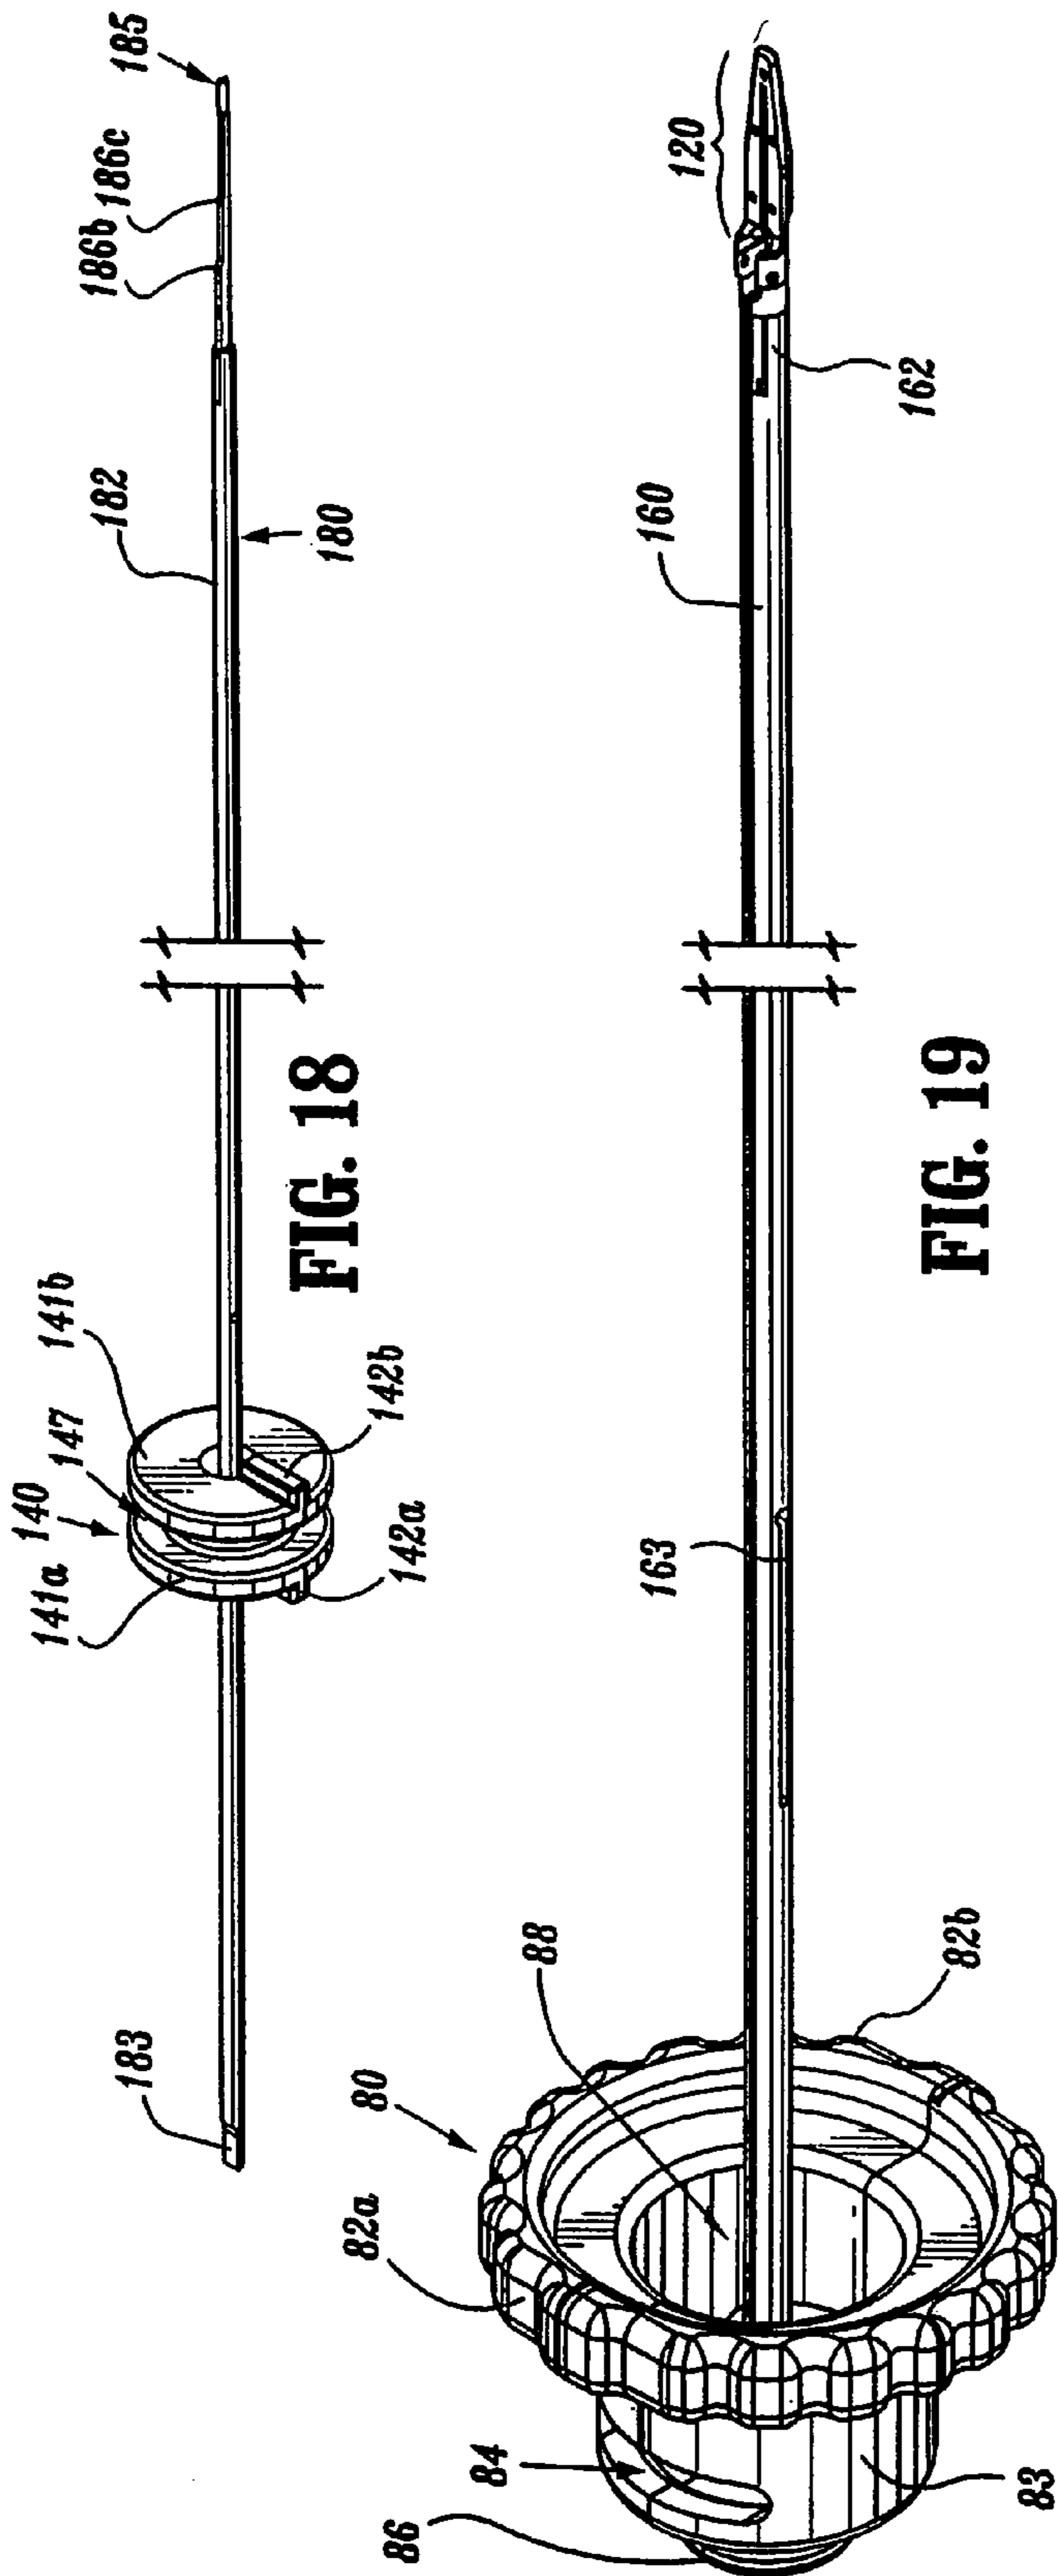


FIG. 18

FIG. 19

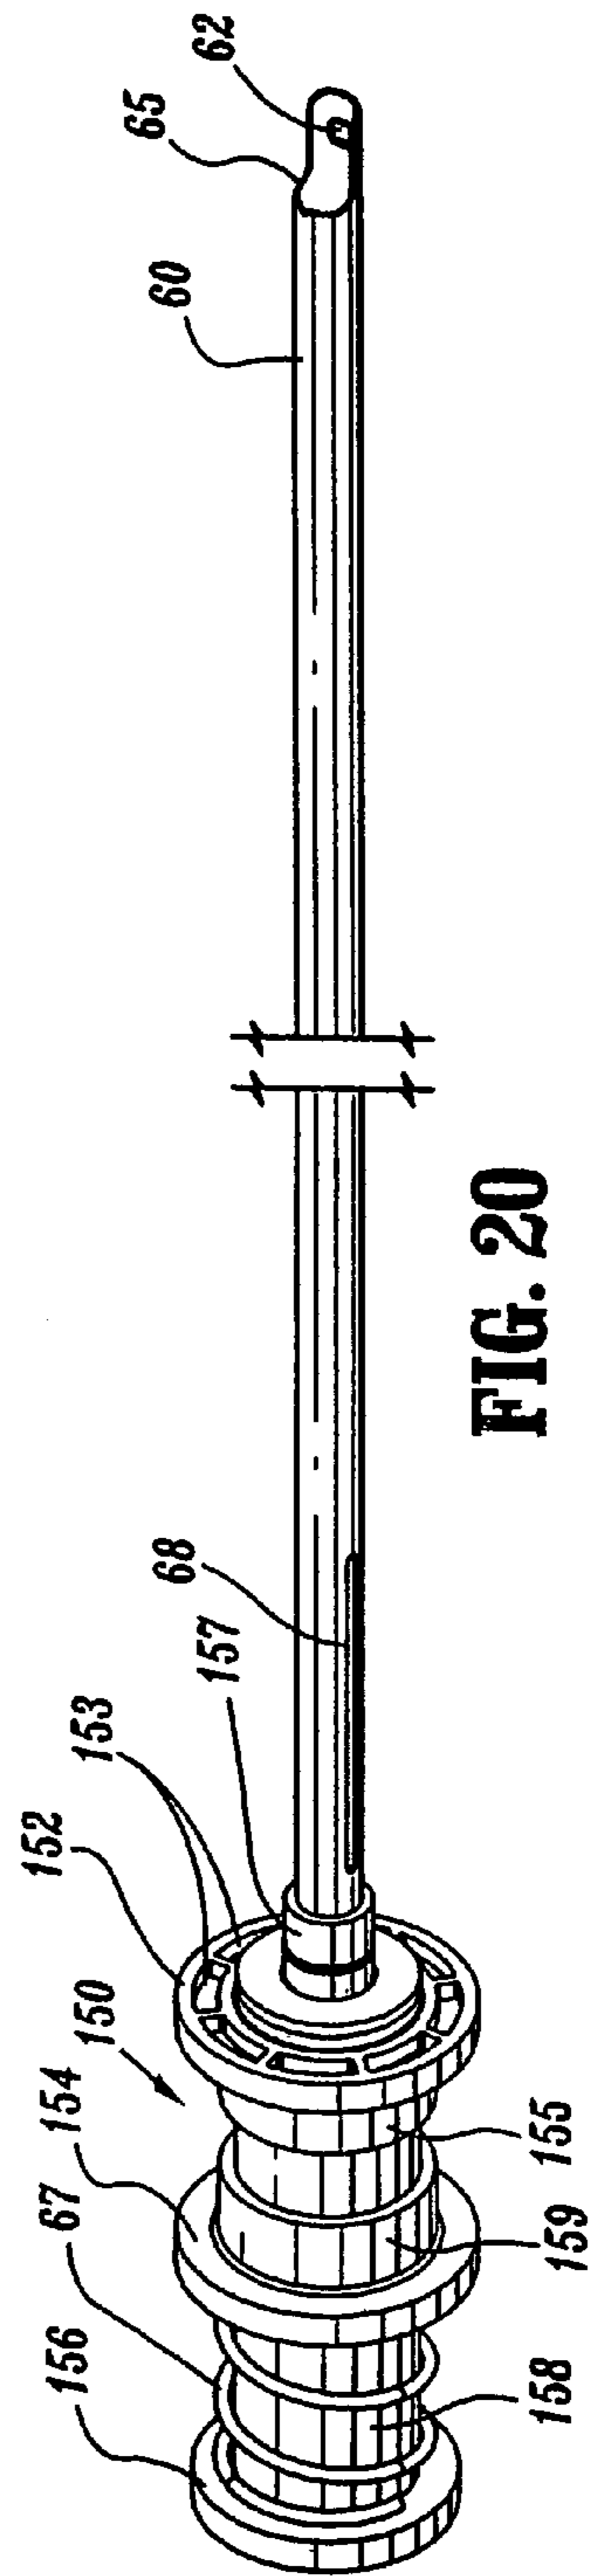


FIG. 20

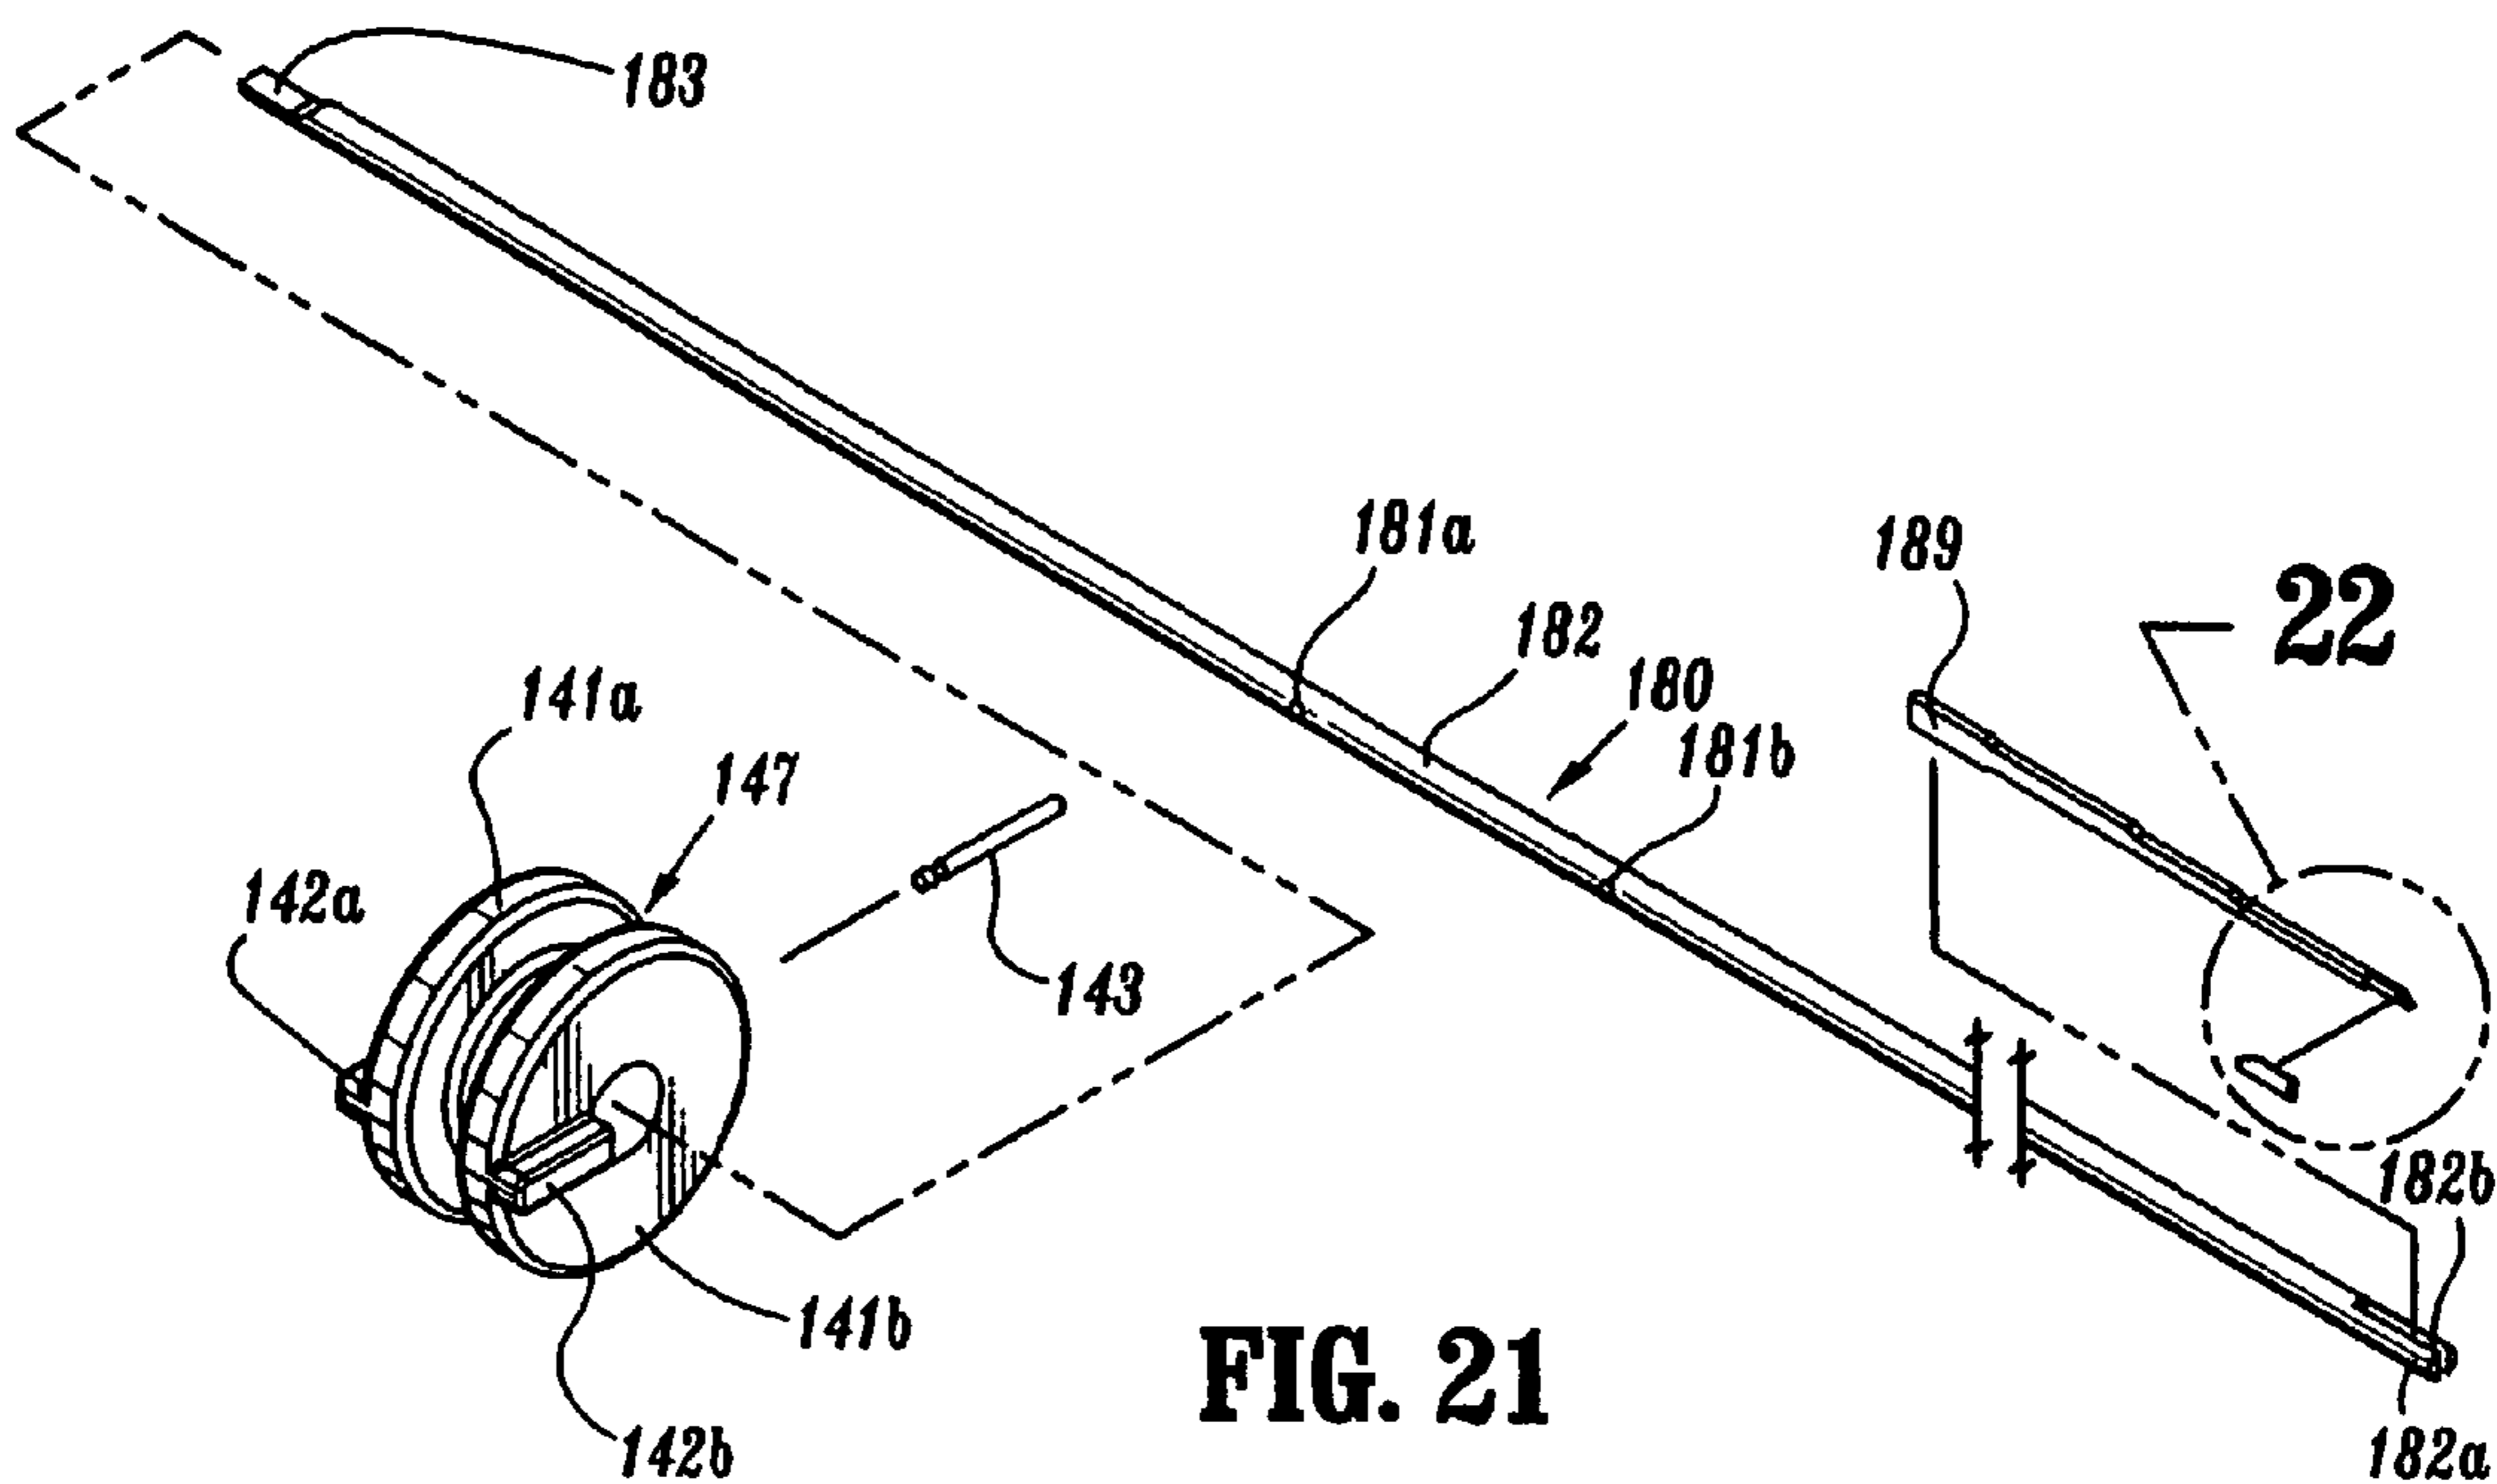


FIG. 21

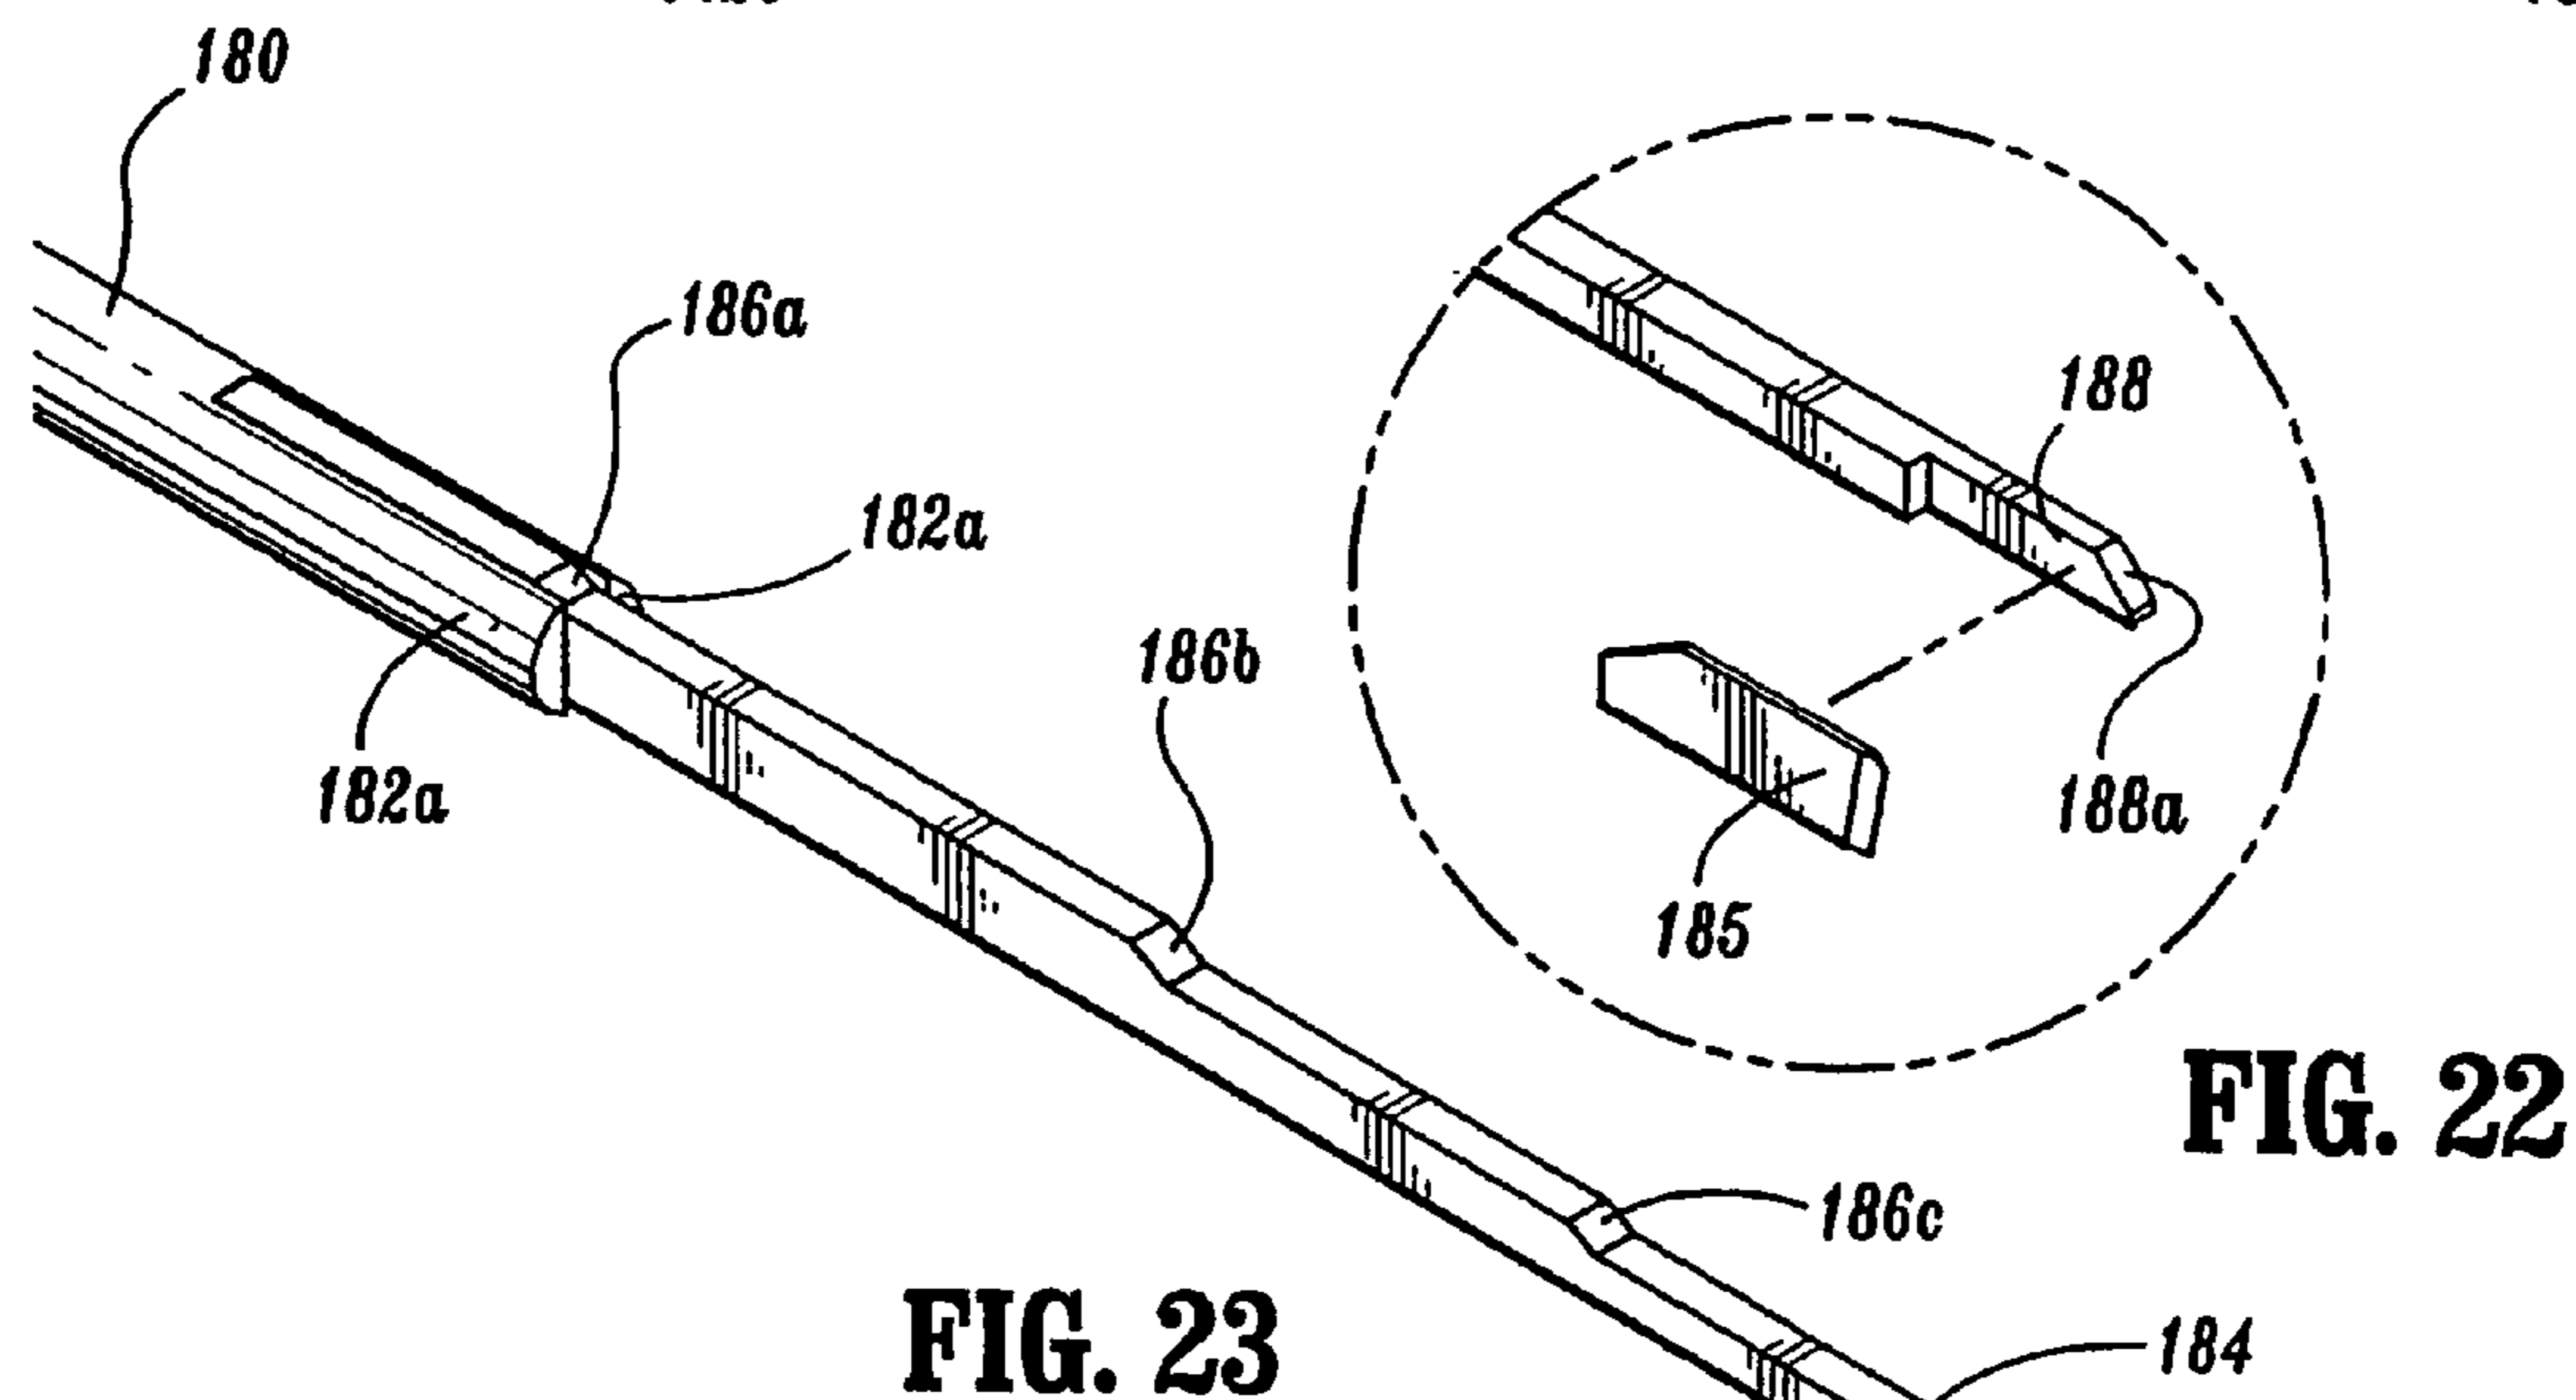


FIG. 22

FIG. 23

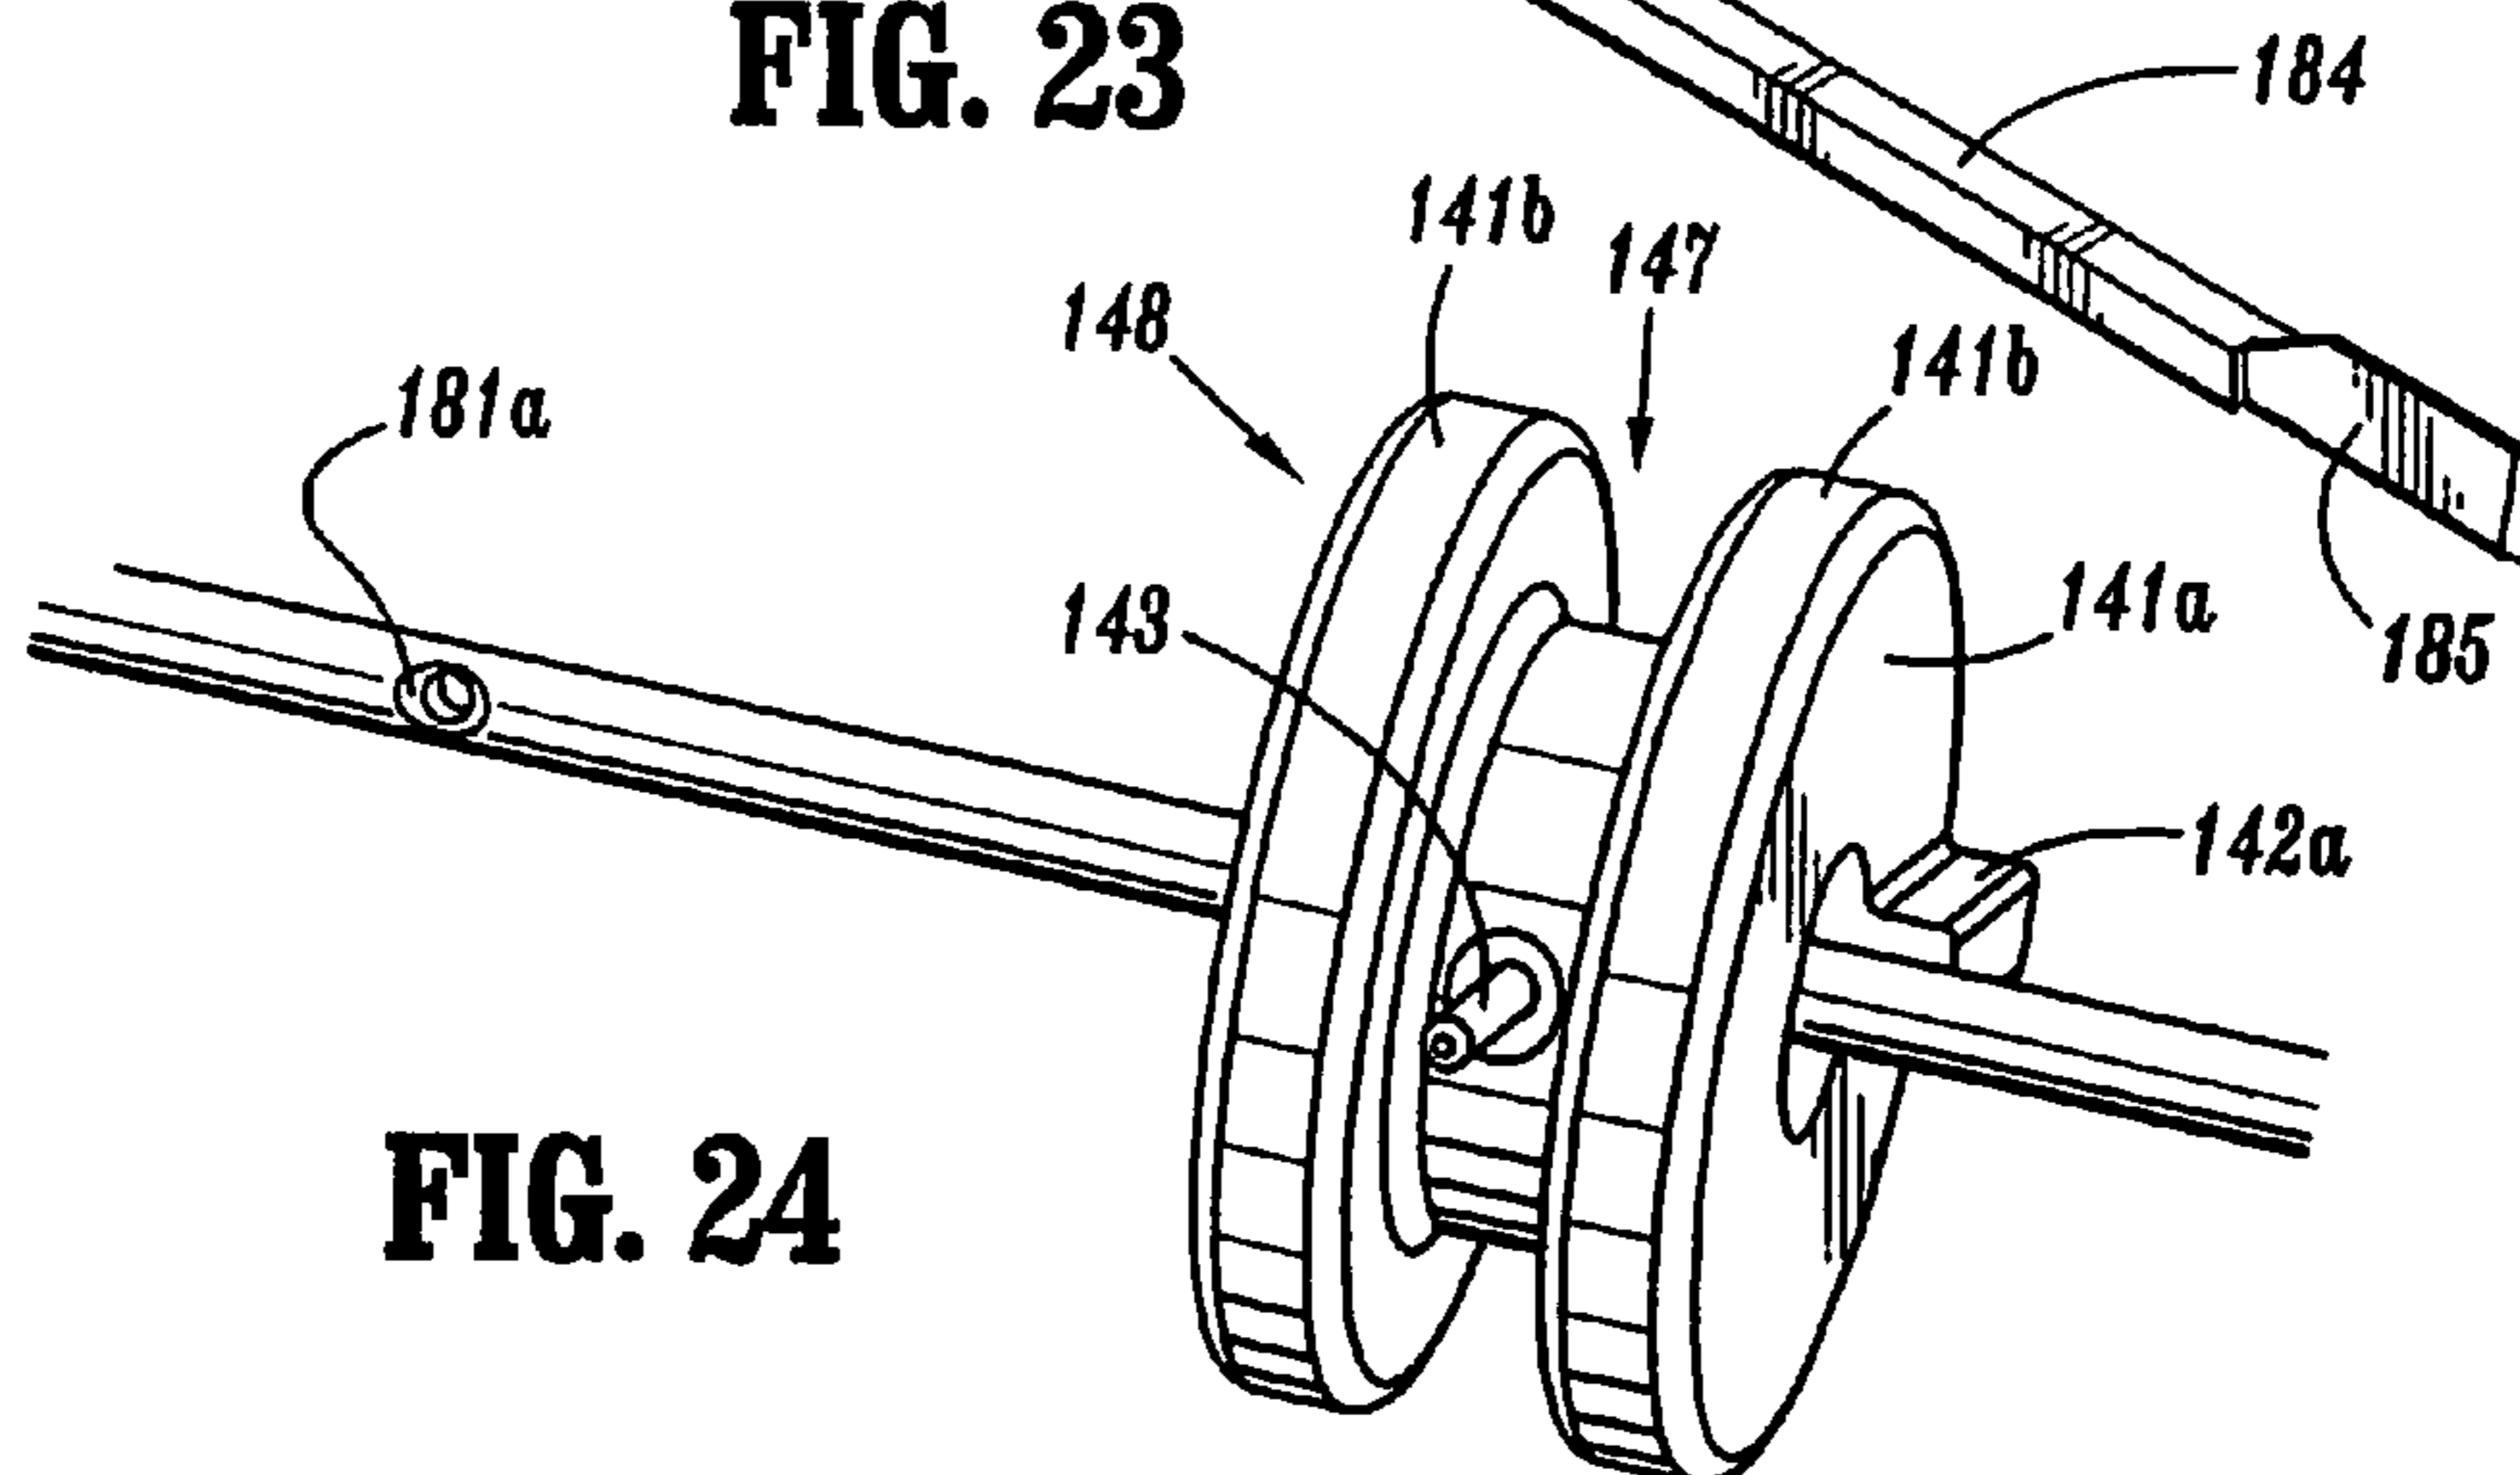


FIG. 24

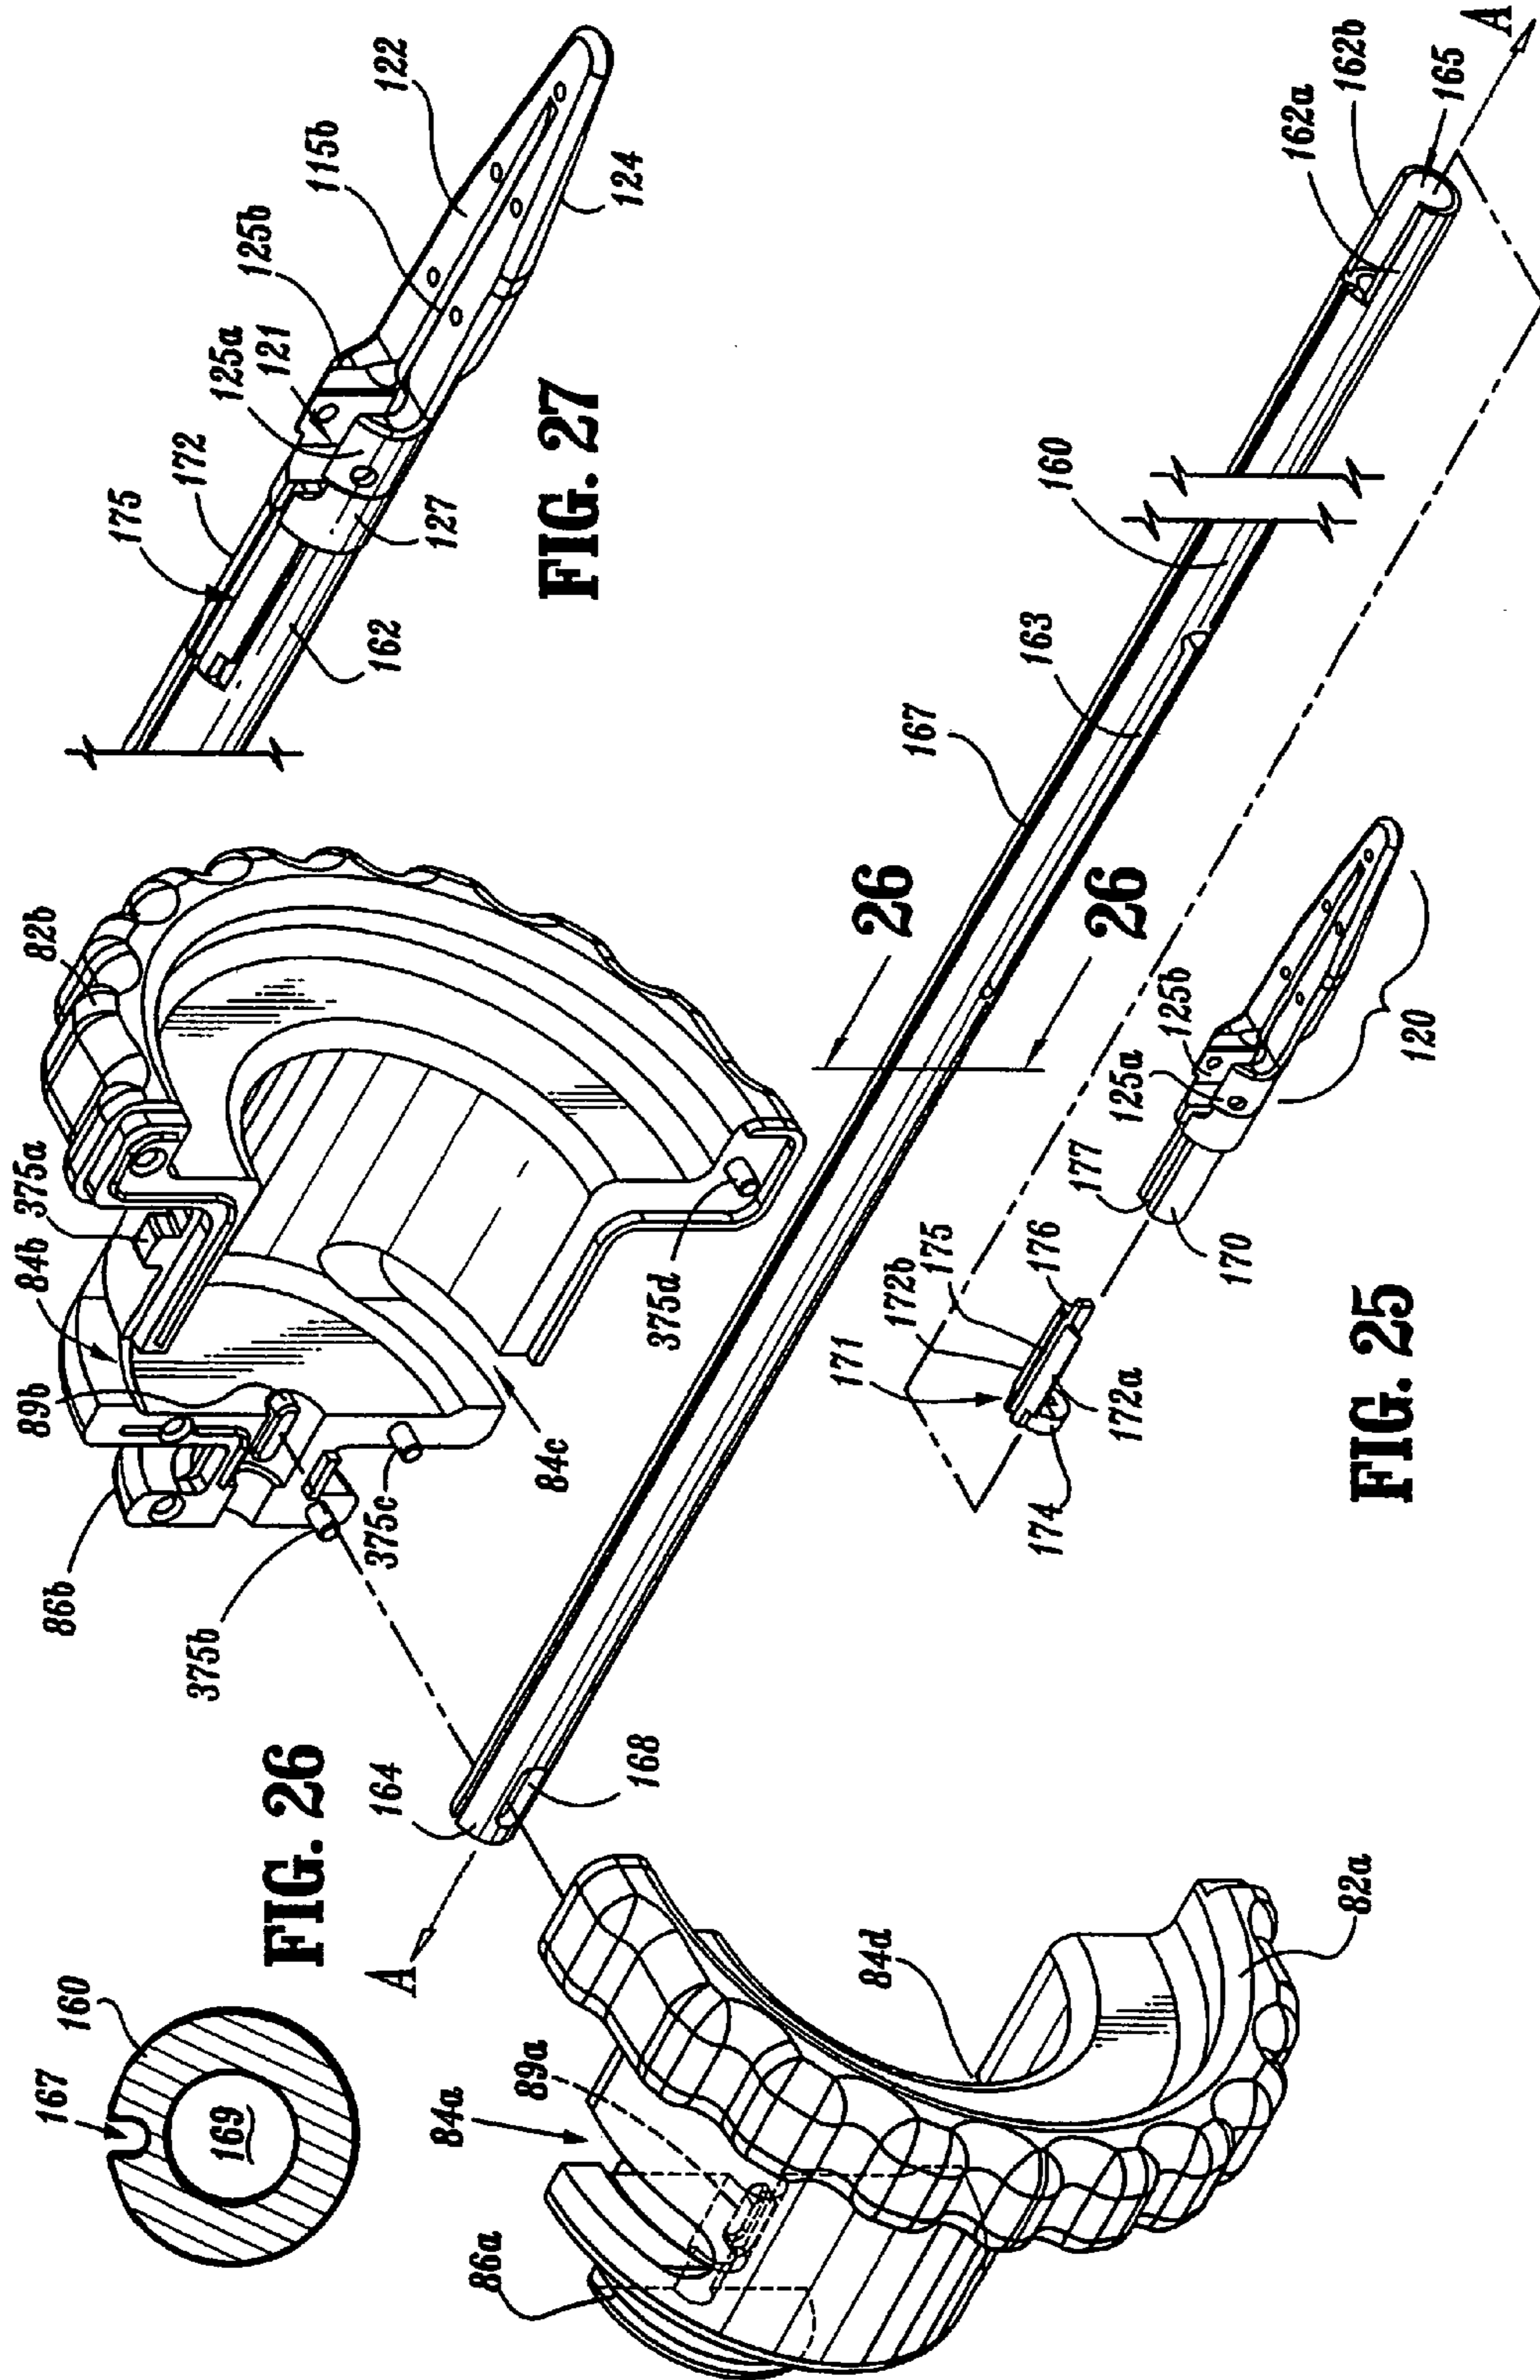


FIG. 27

FIG. 25

FIG. 26

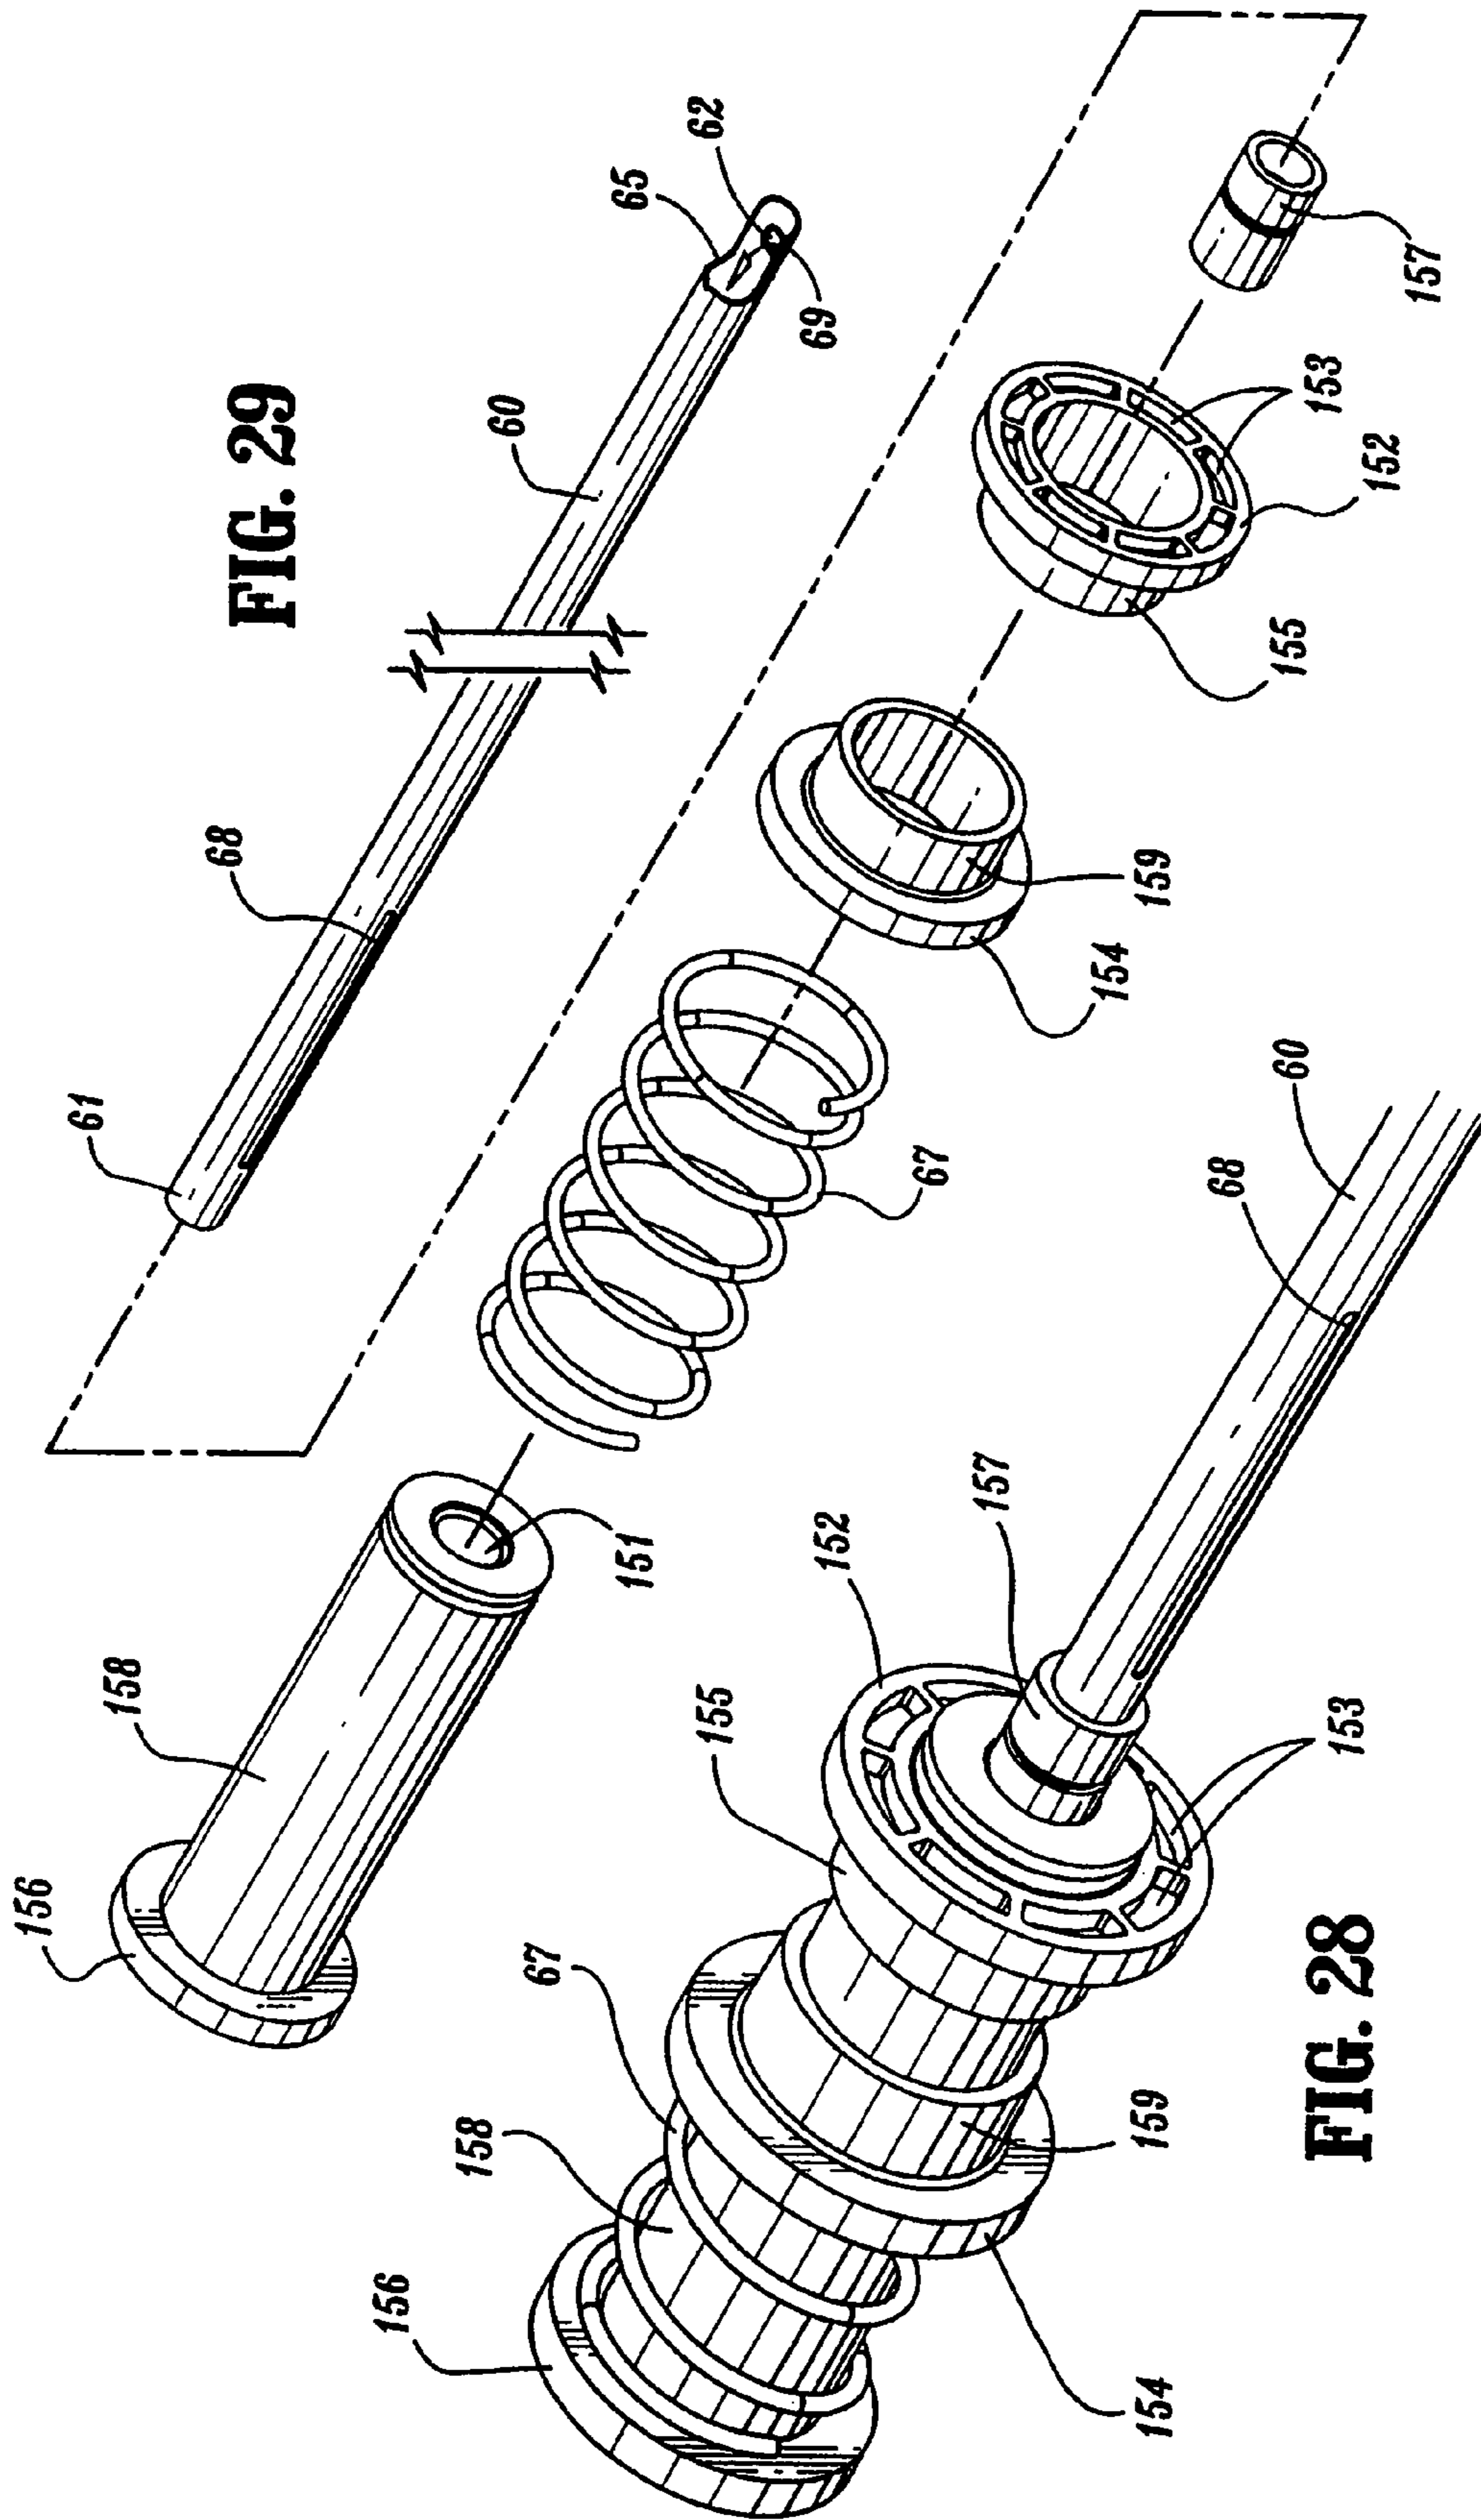


FIG. 29

FIG. 28

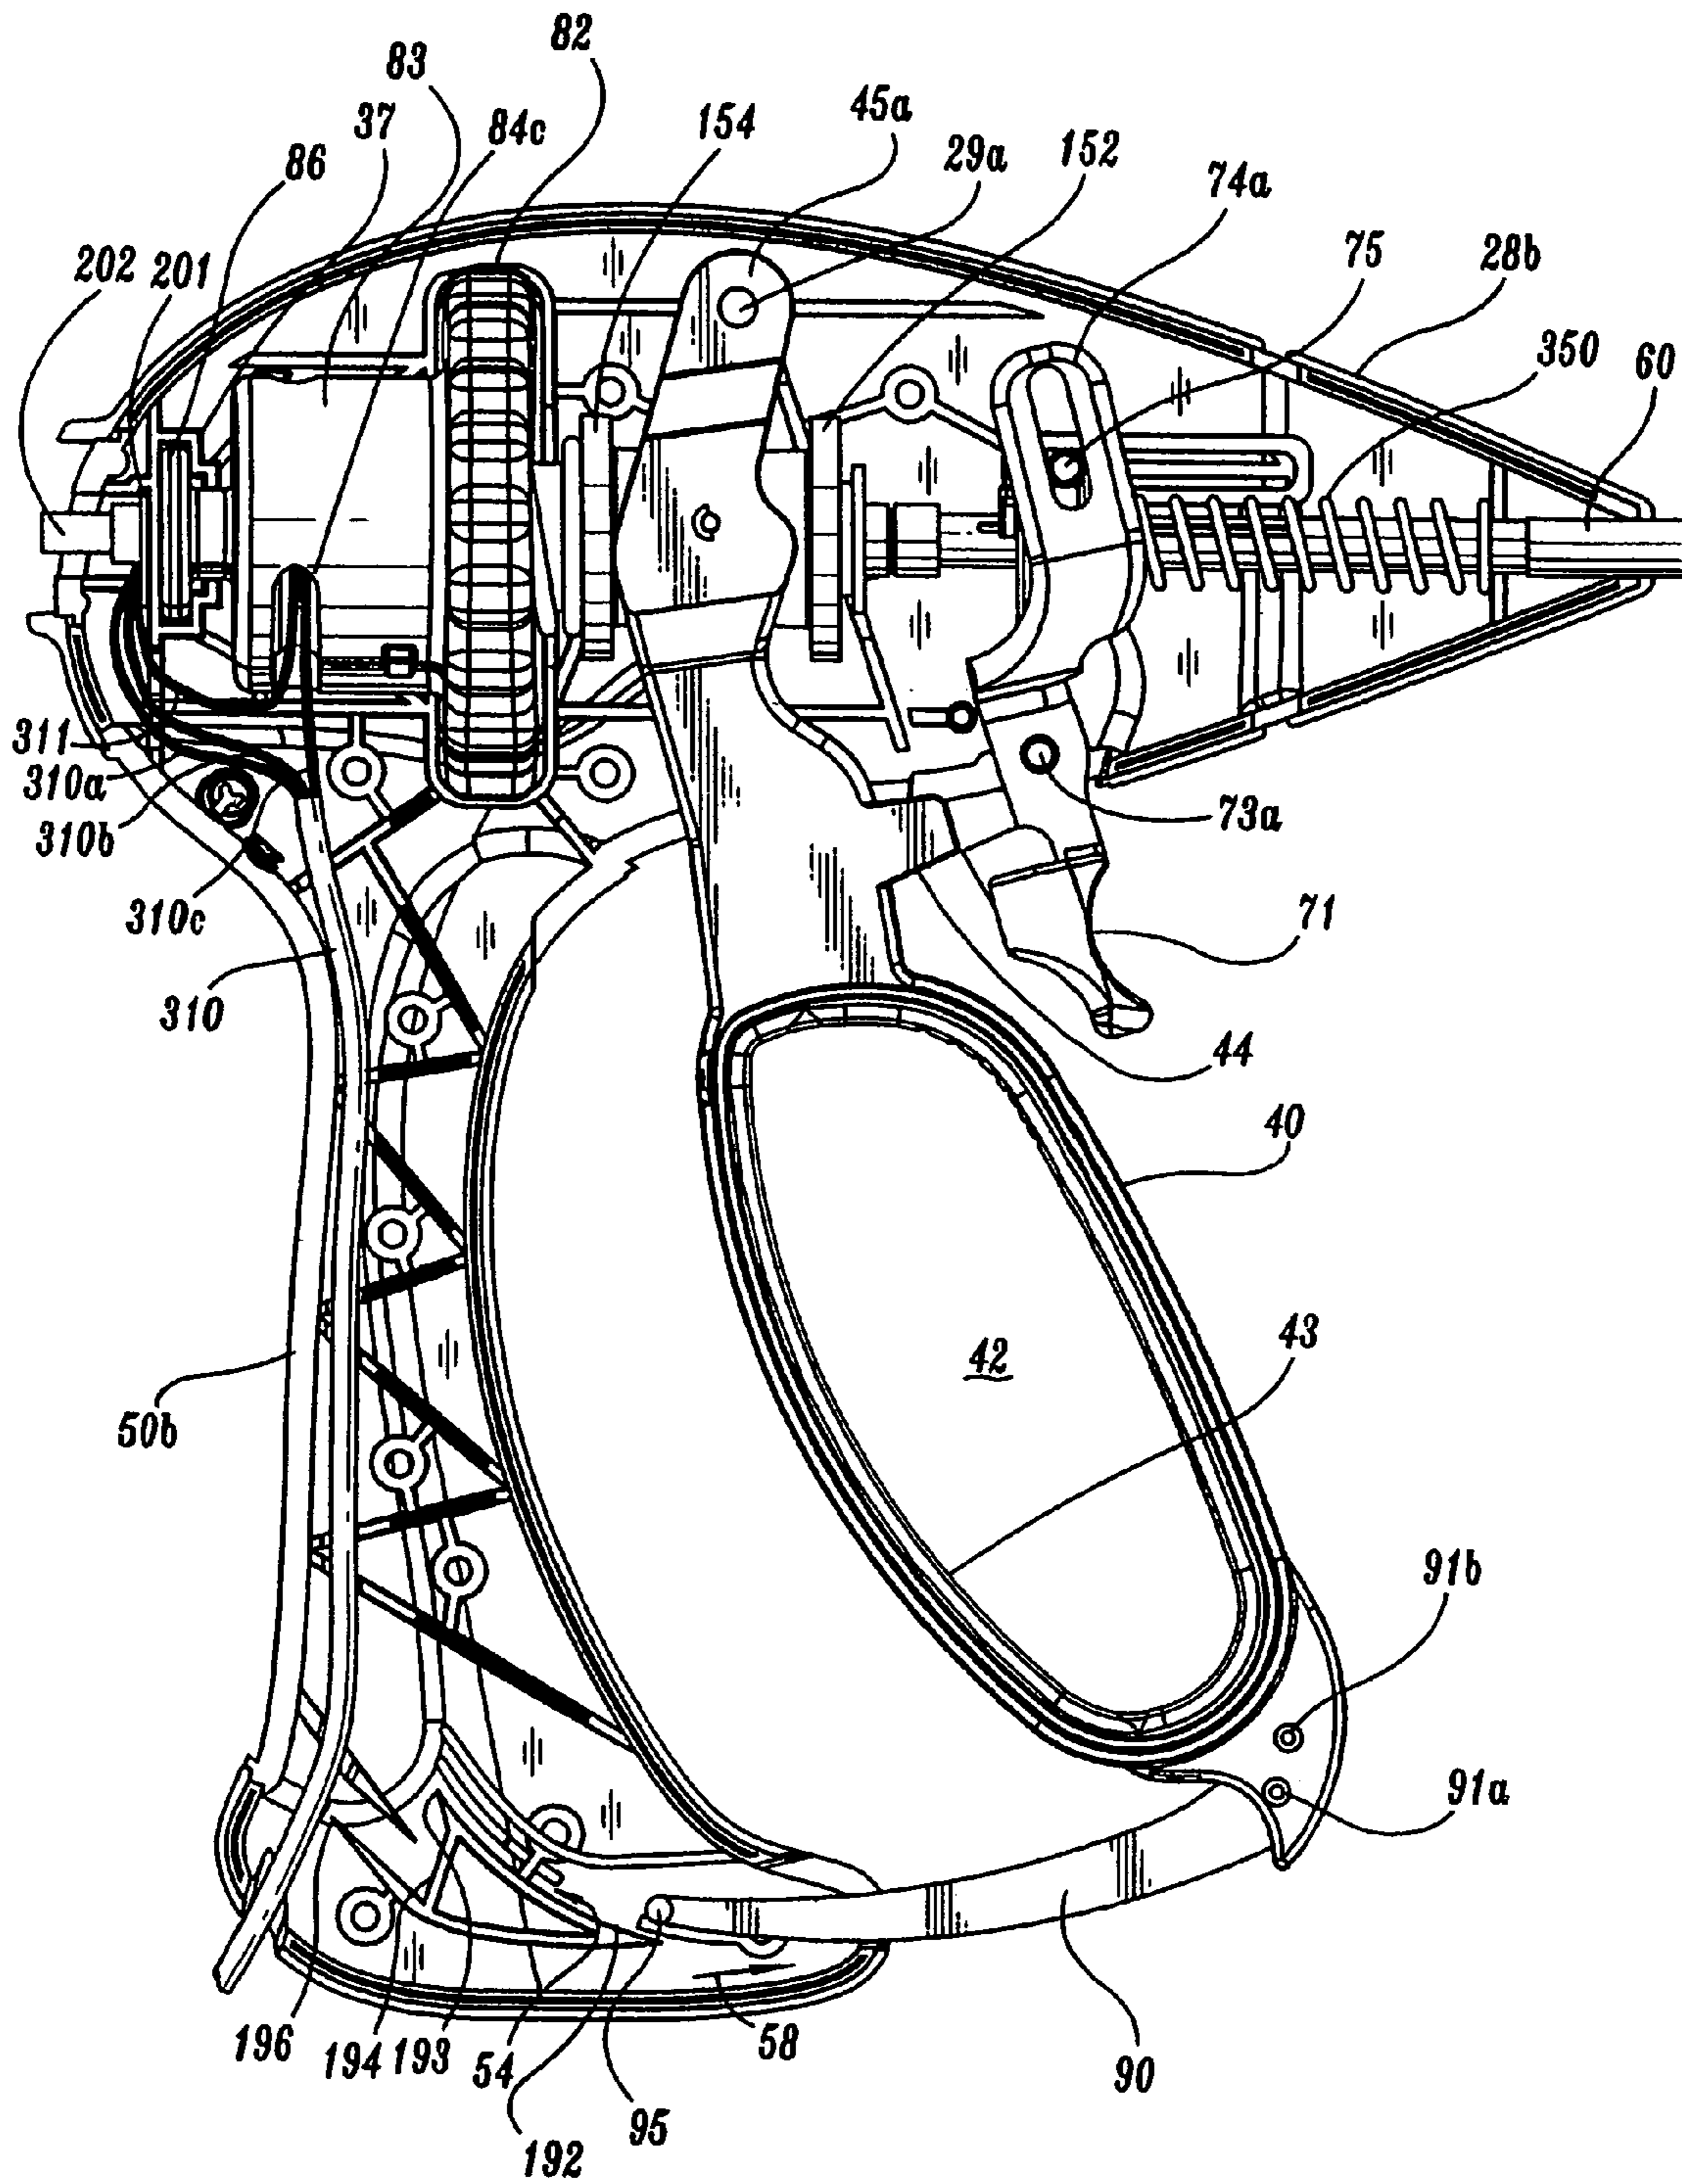


FIG. 30

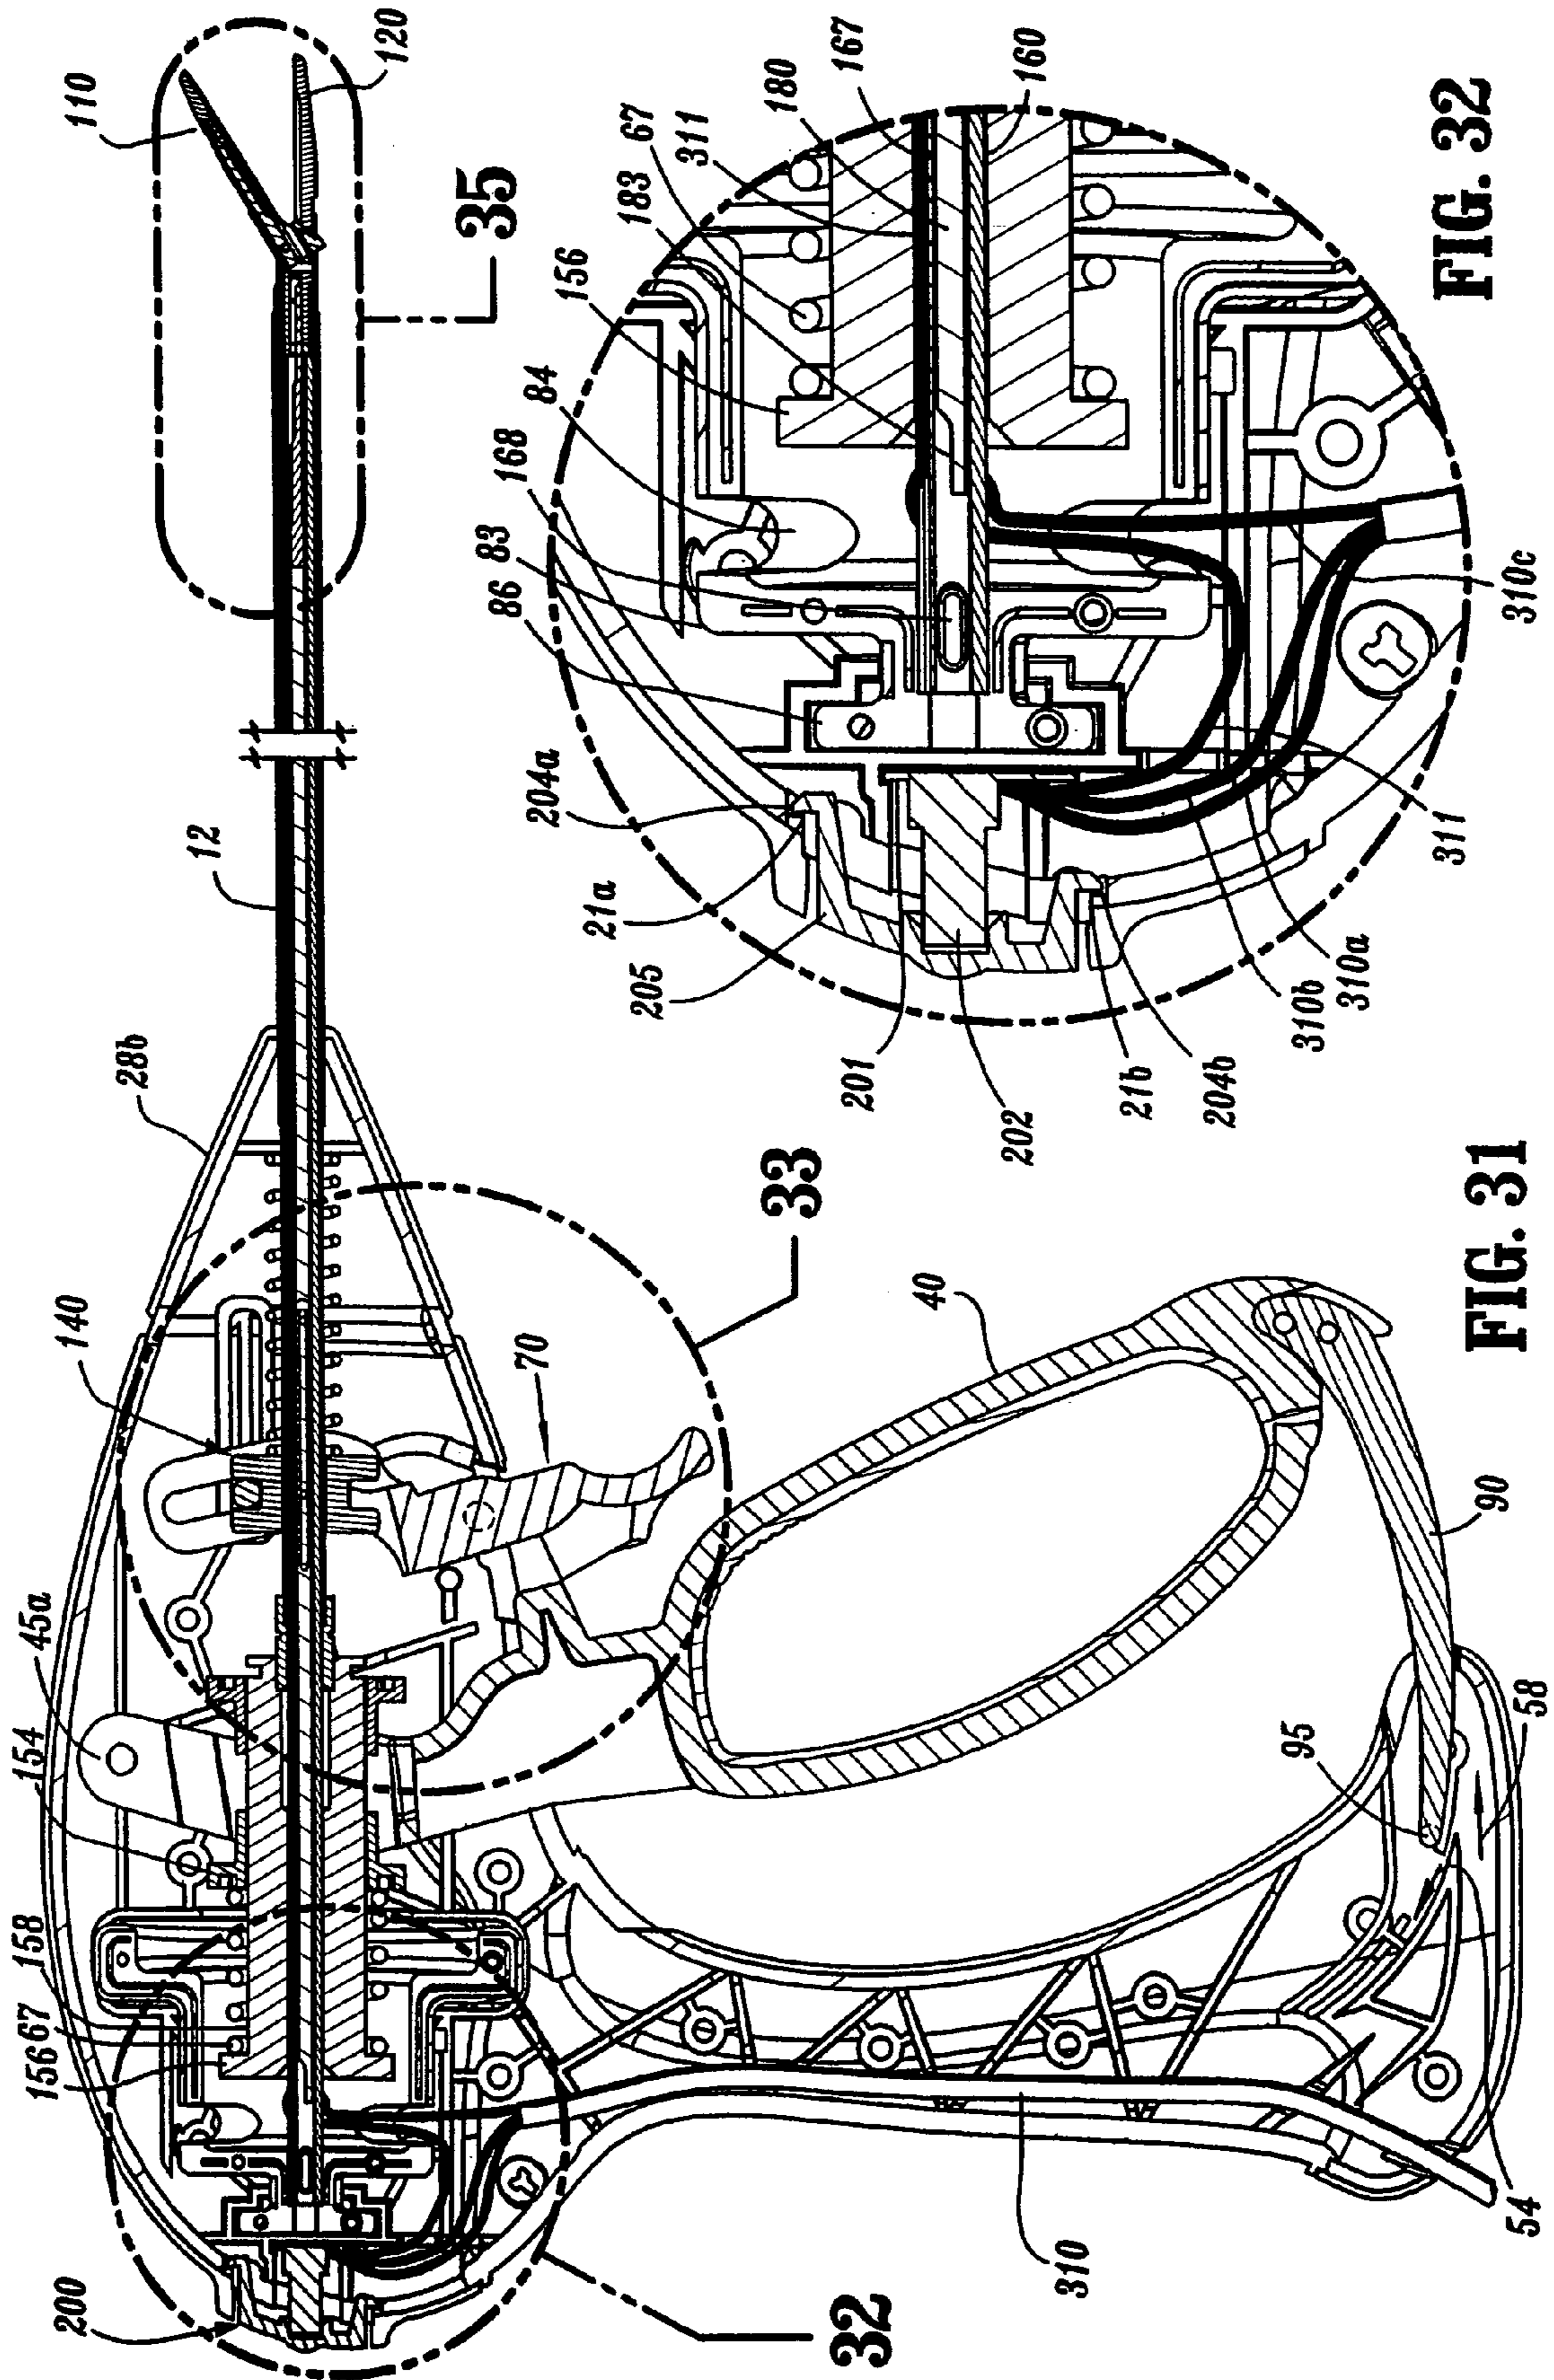


FIG. 32

FIG. 31

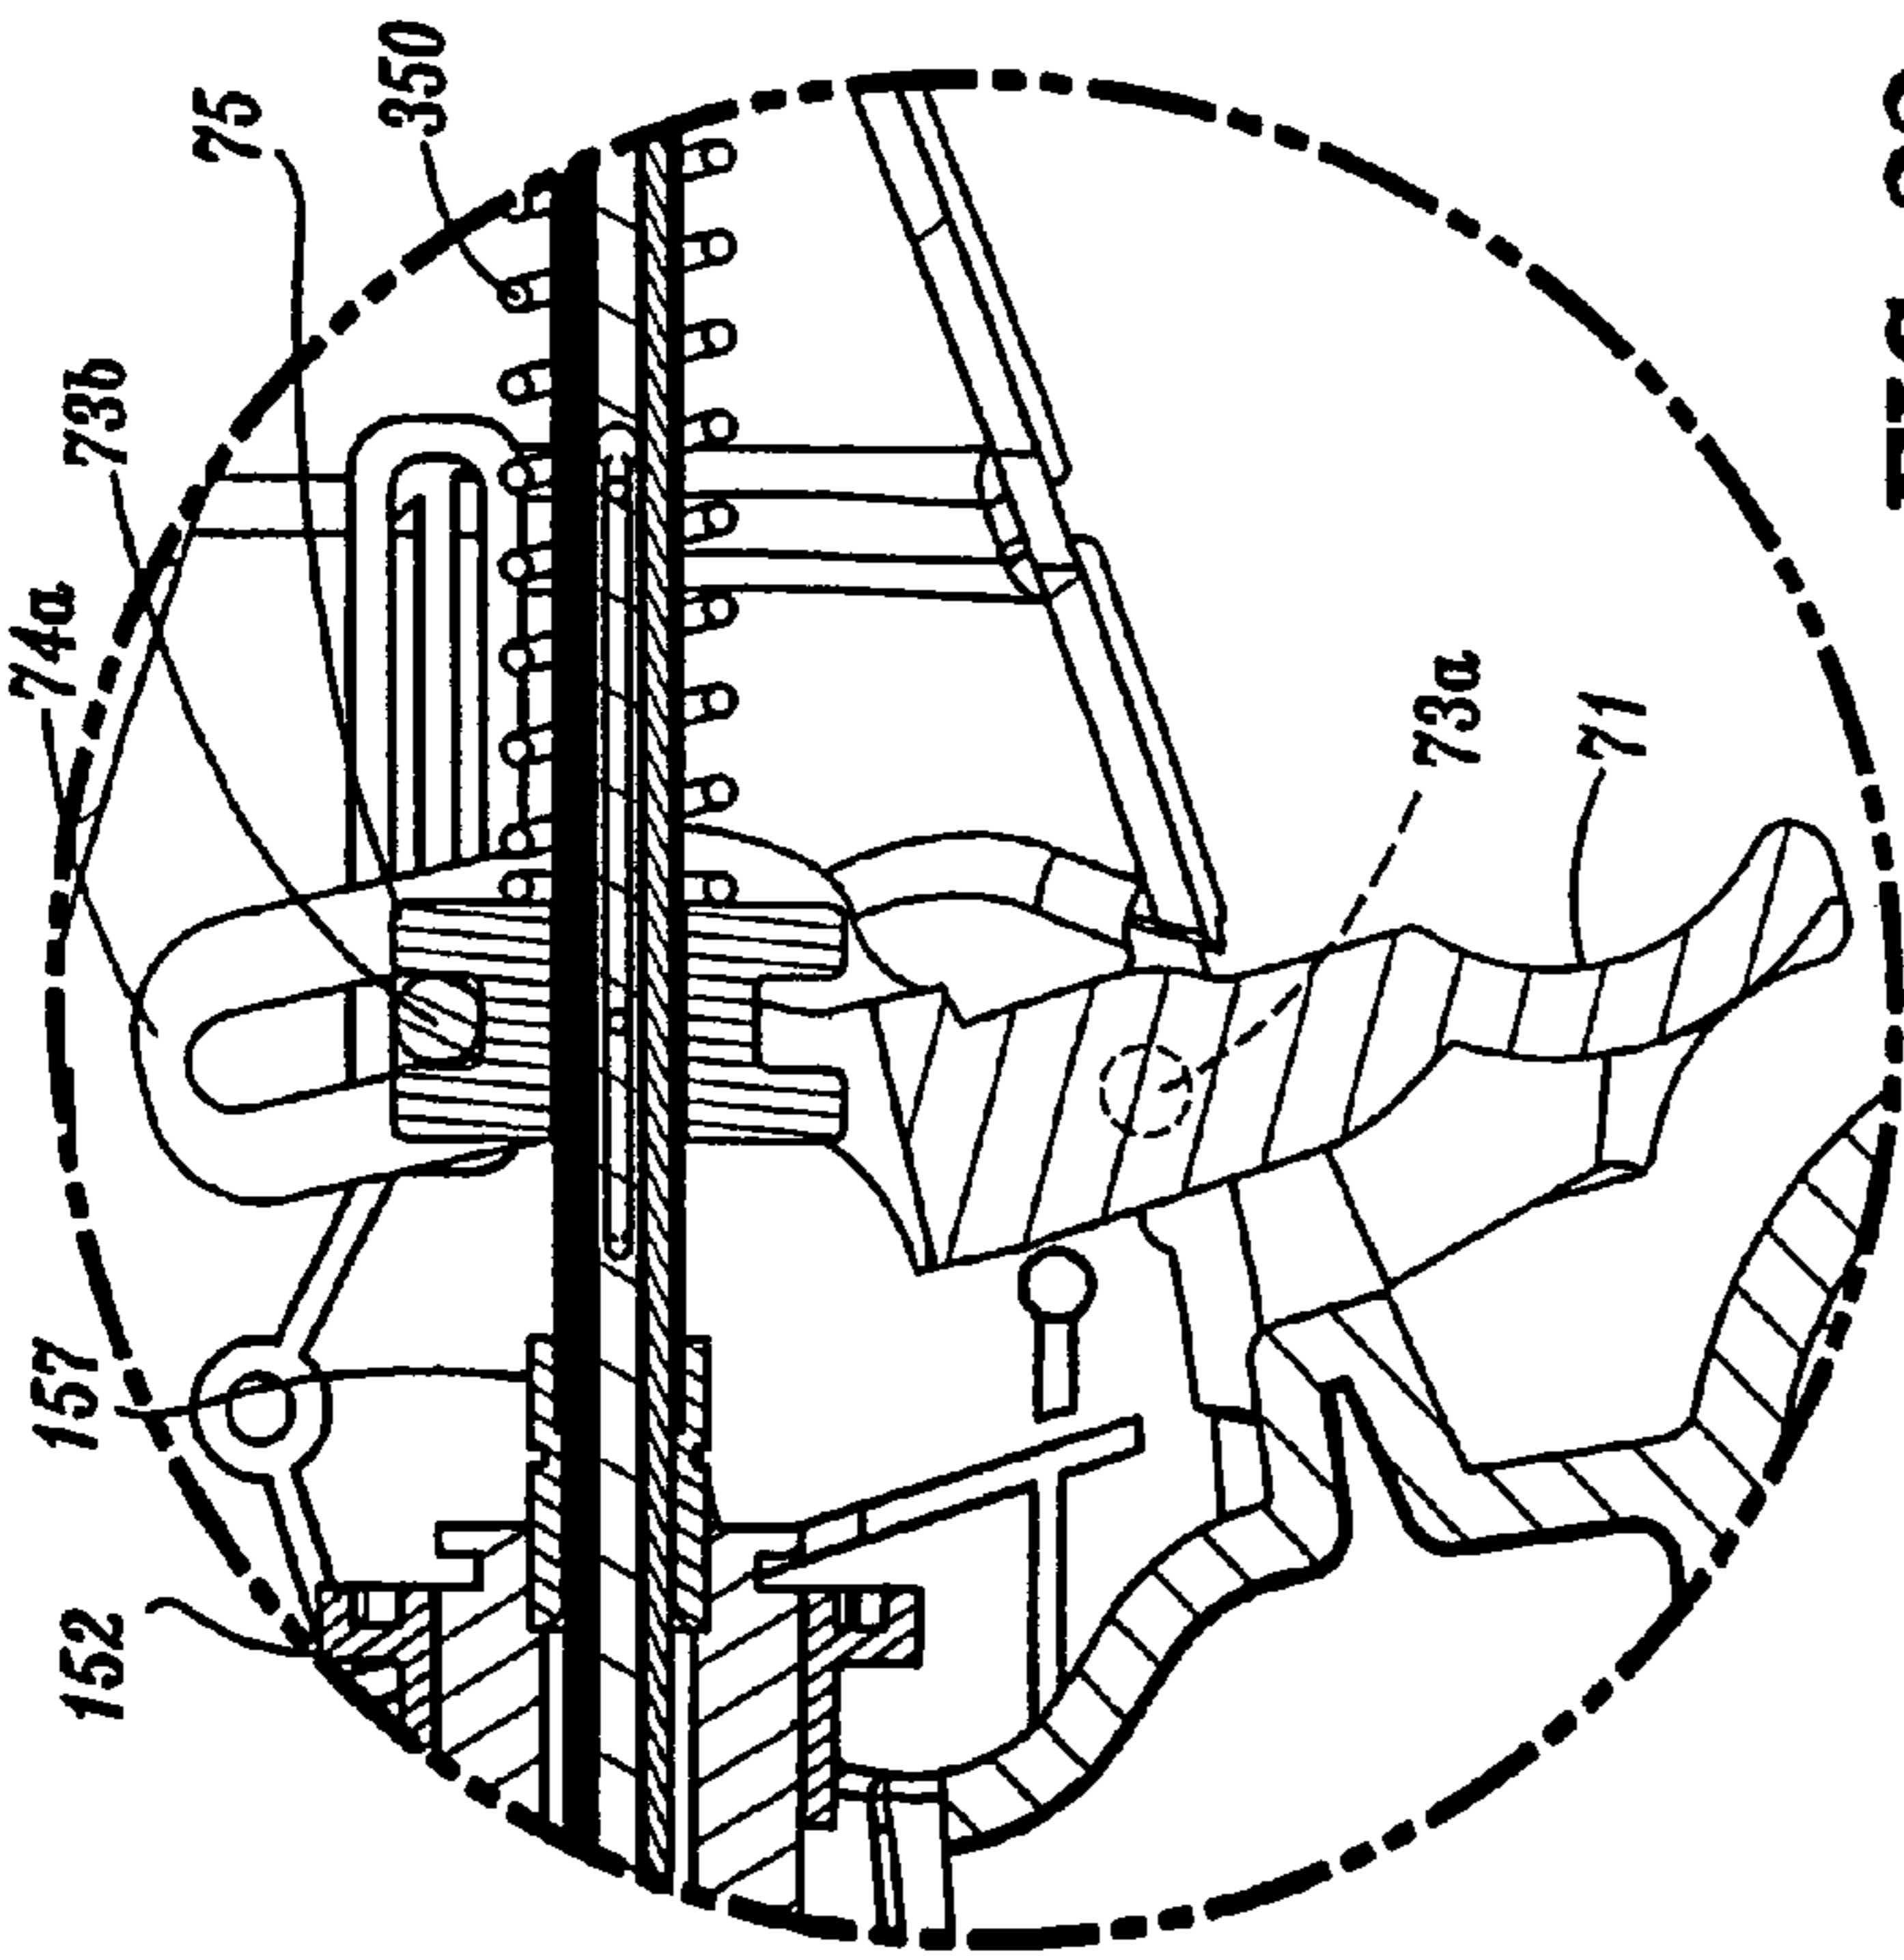


FIG. 33

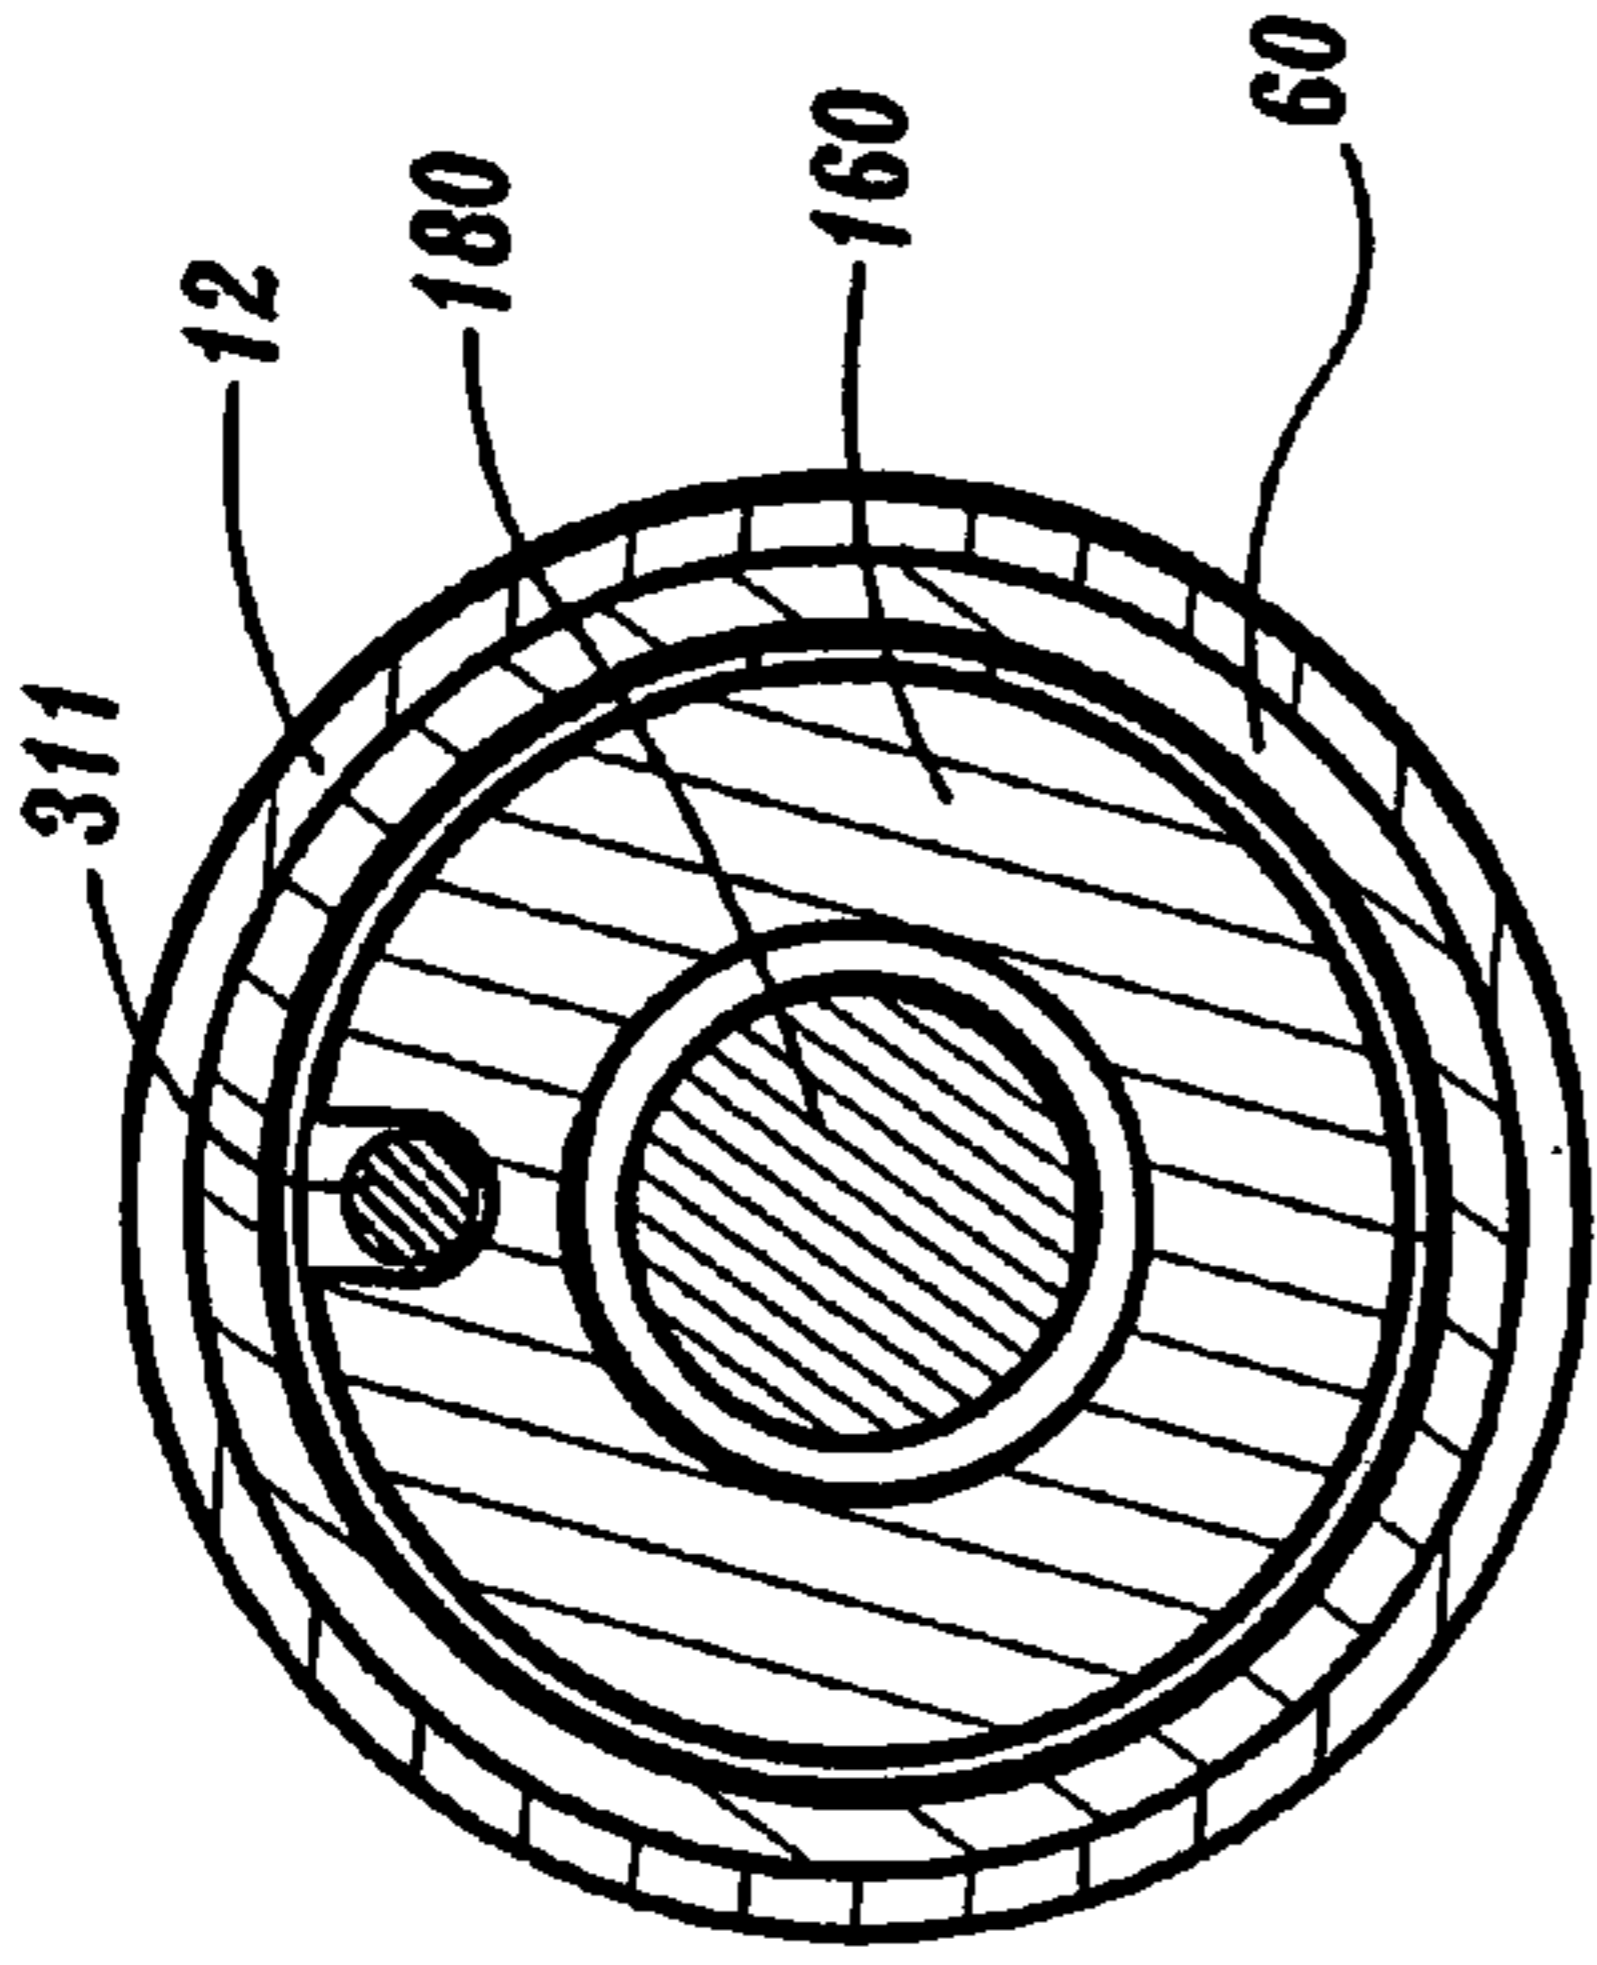


FIG. 34

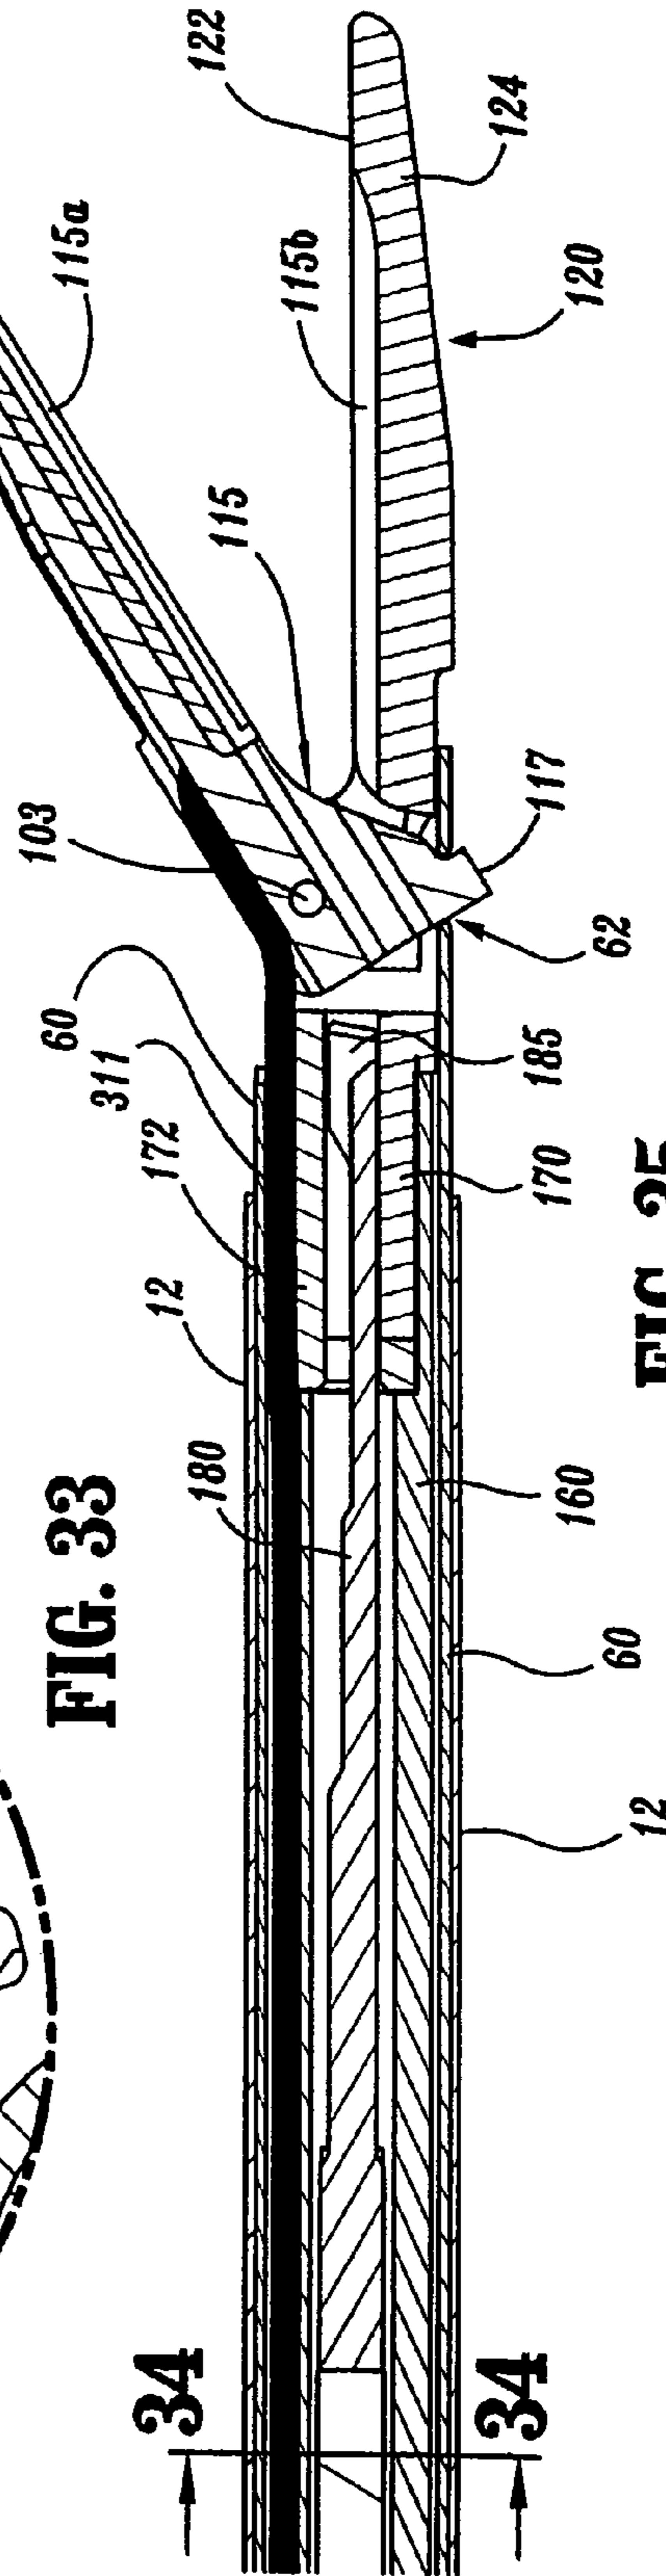


FIG. 35

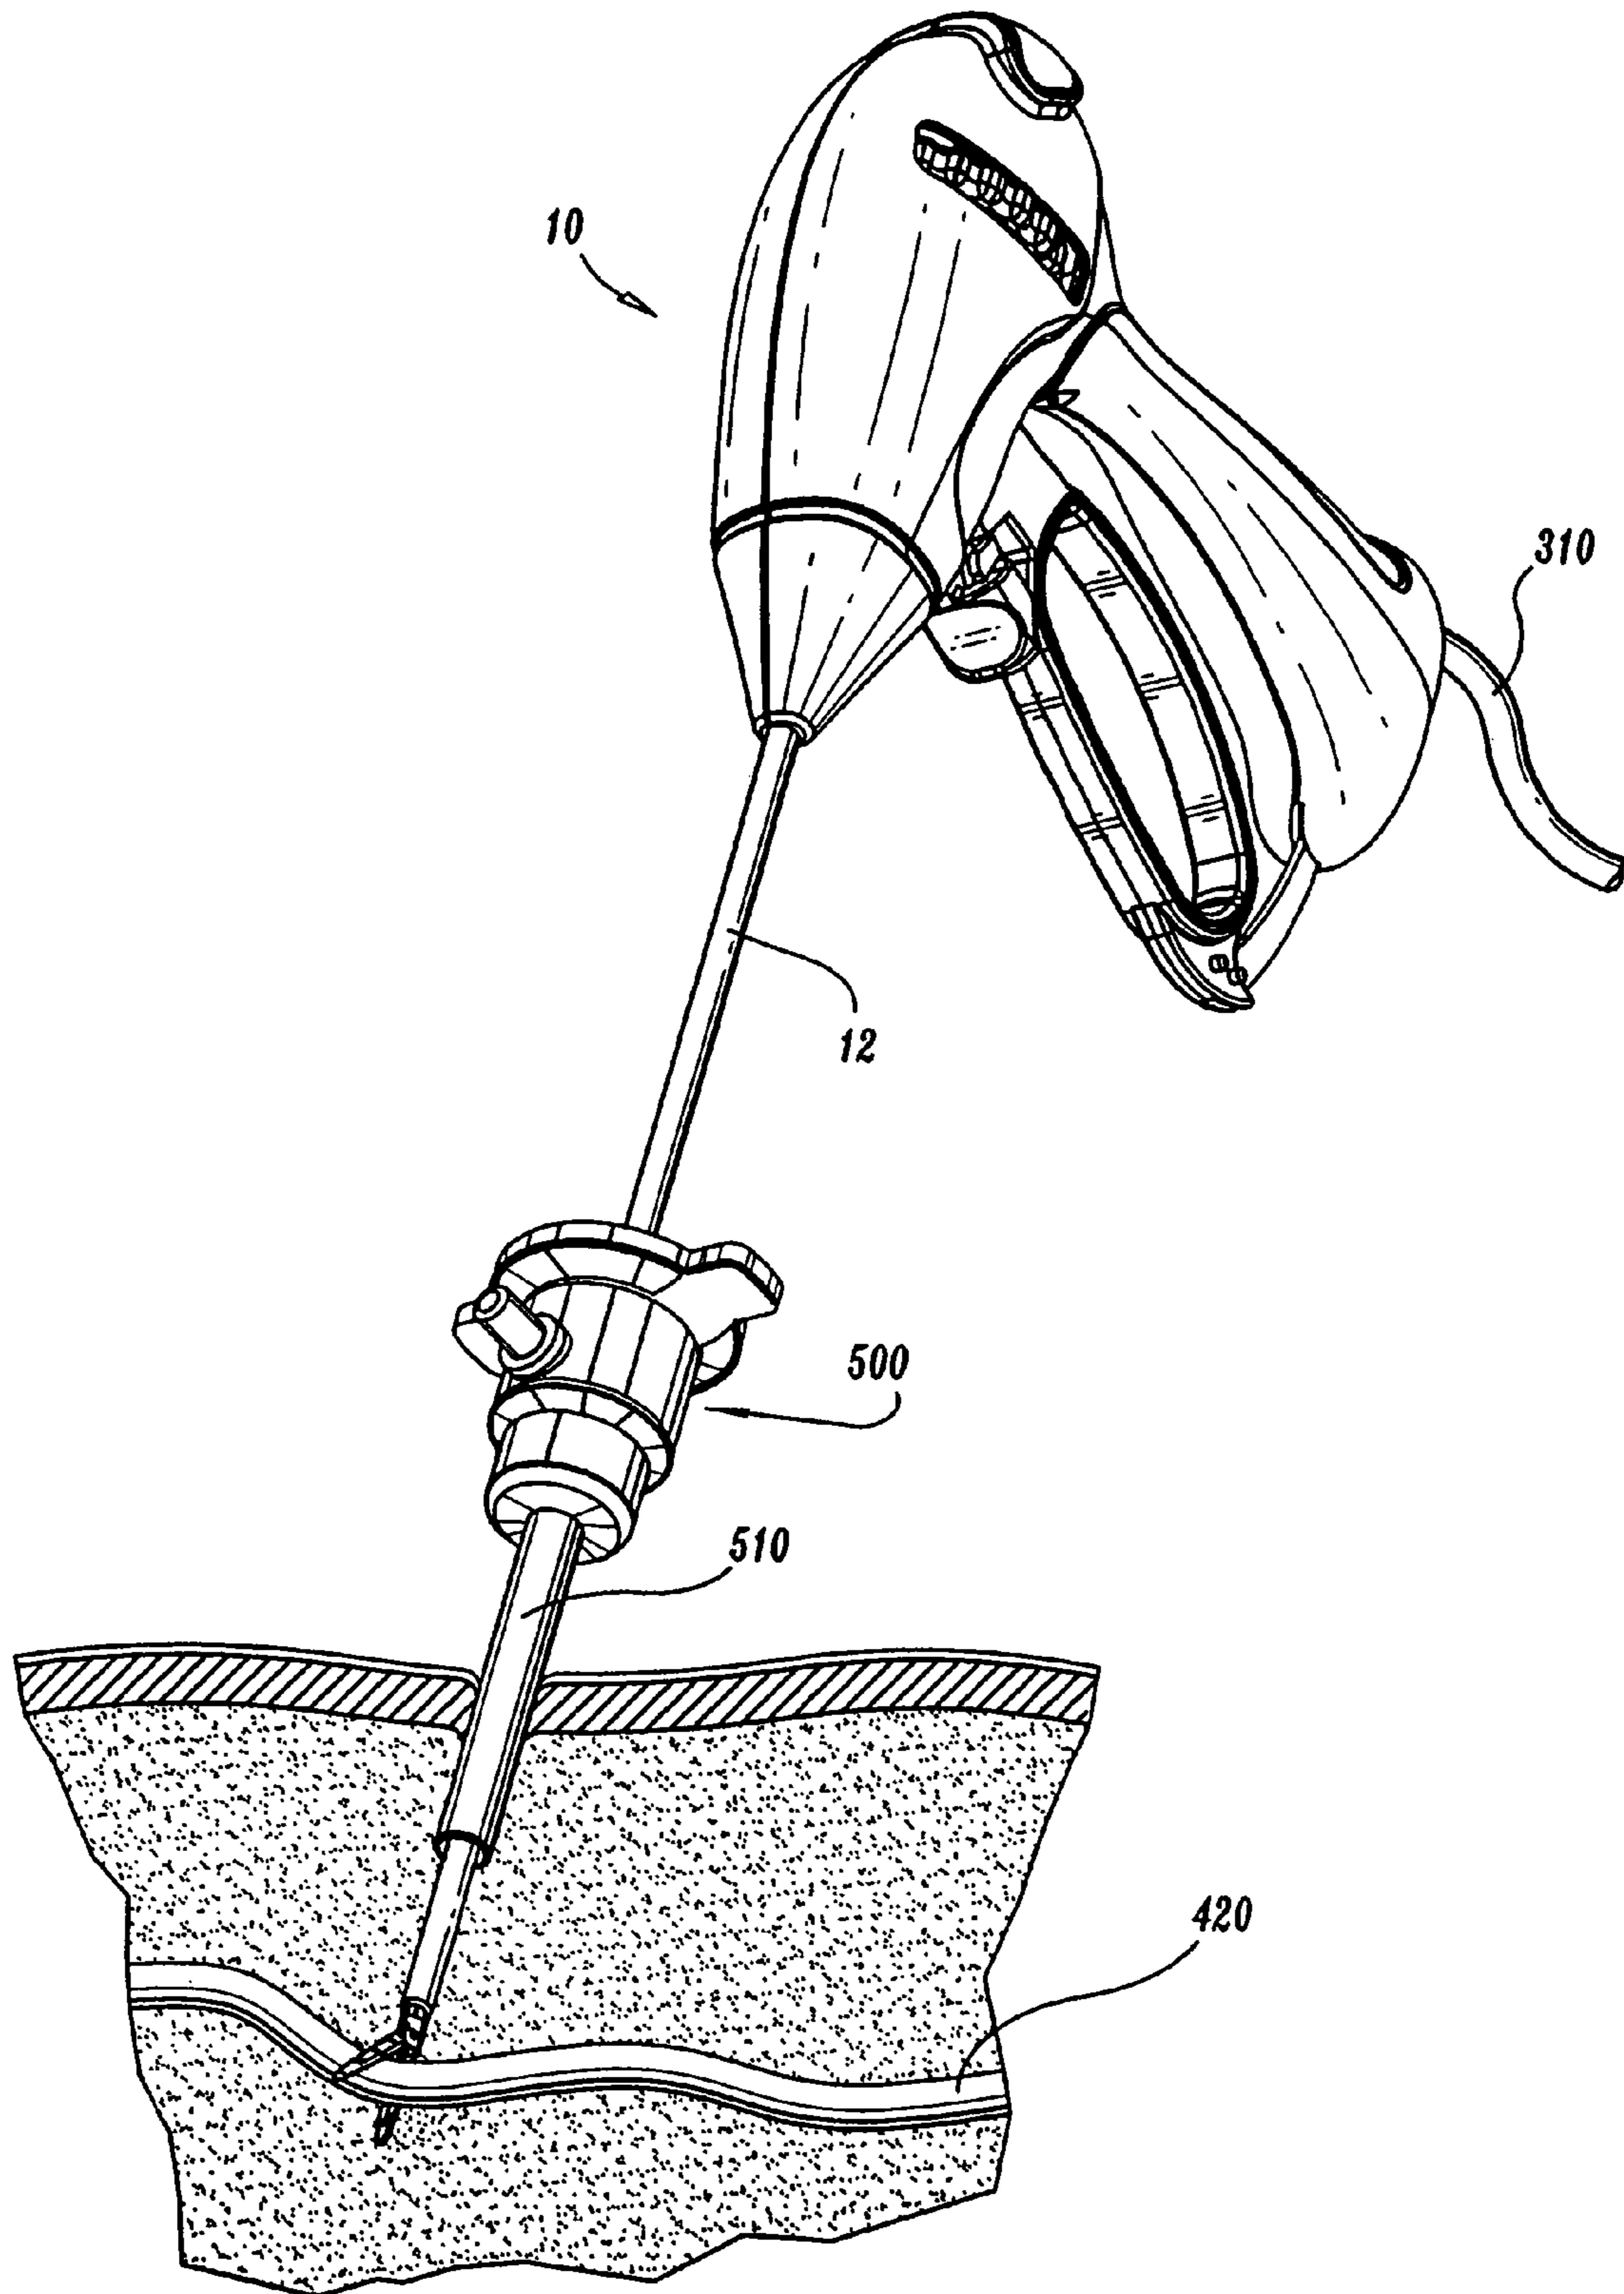


FIG. 36

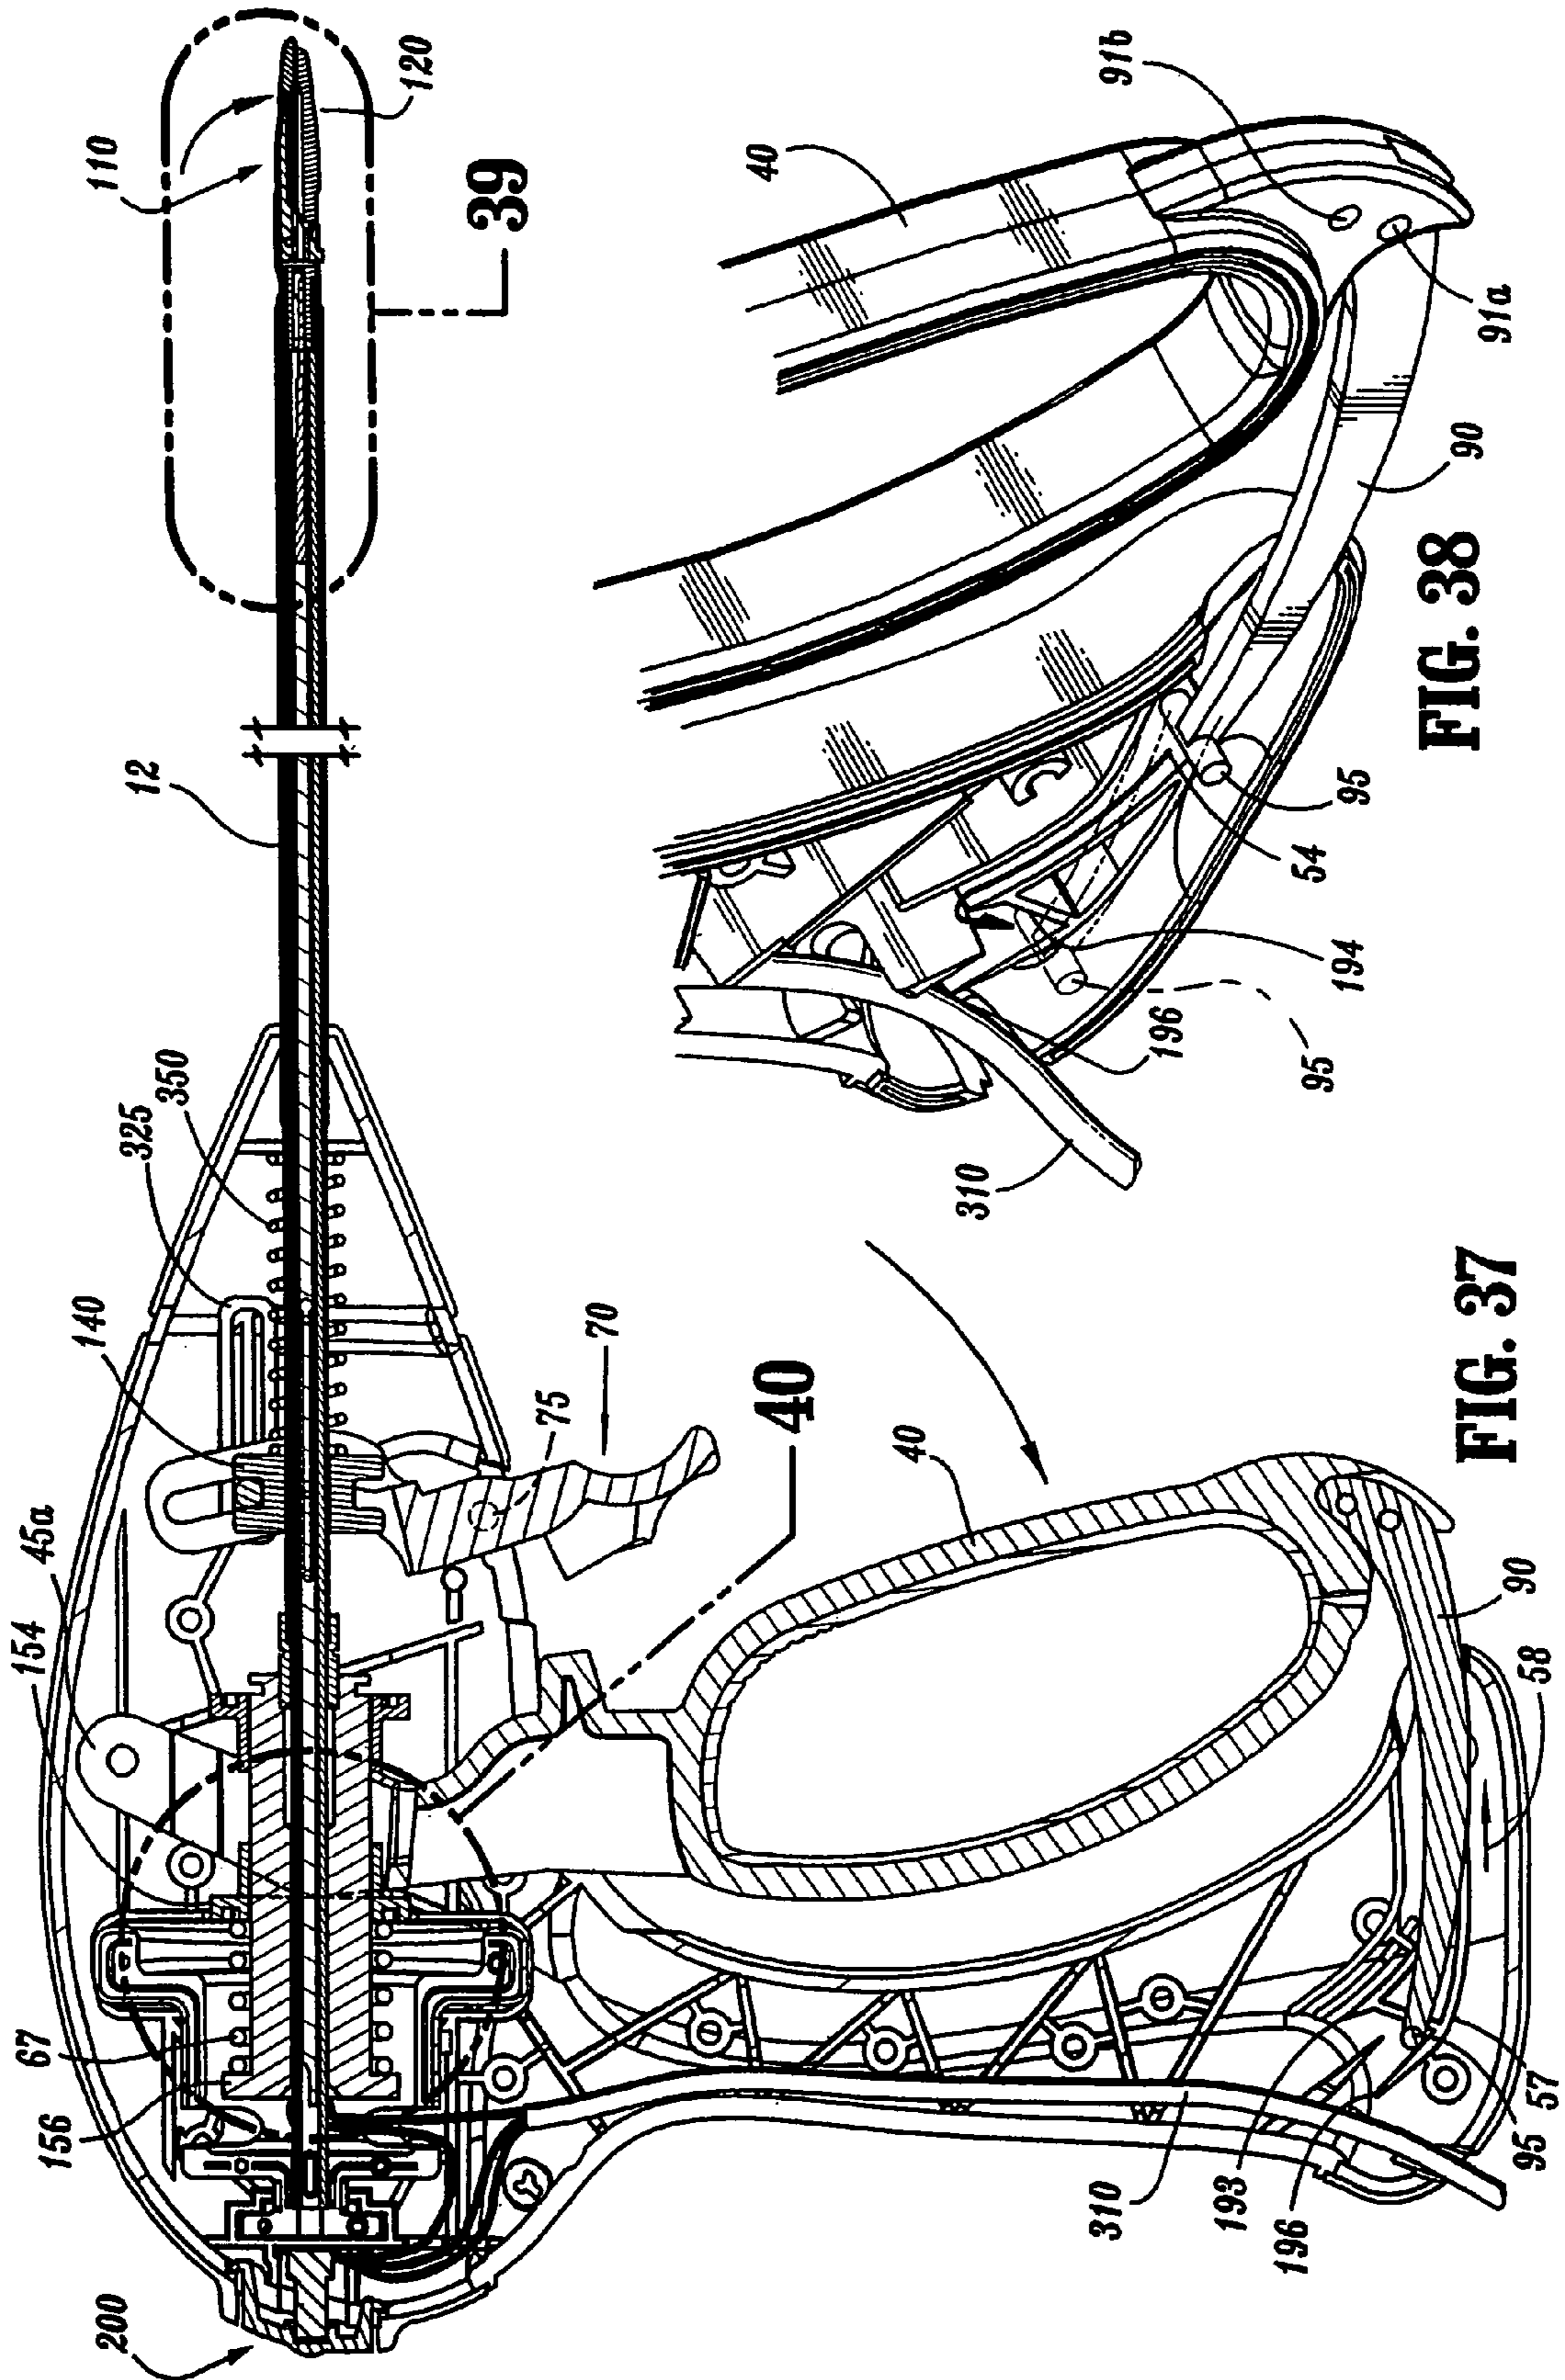


FIG. 38

FIG. 37

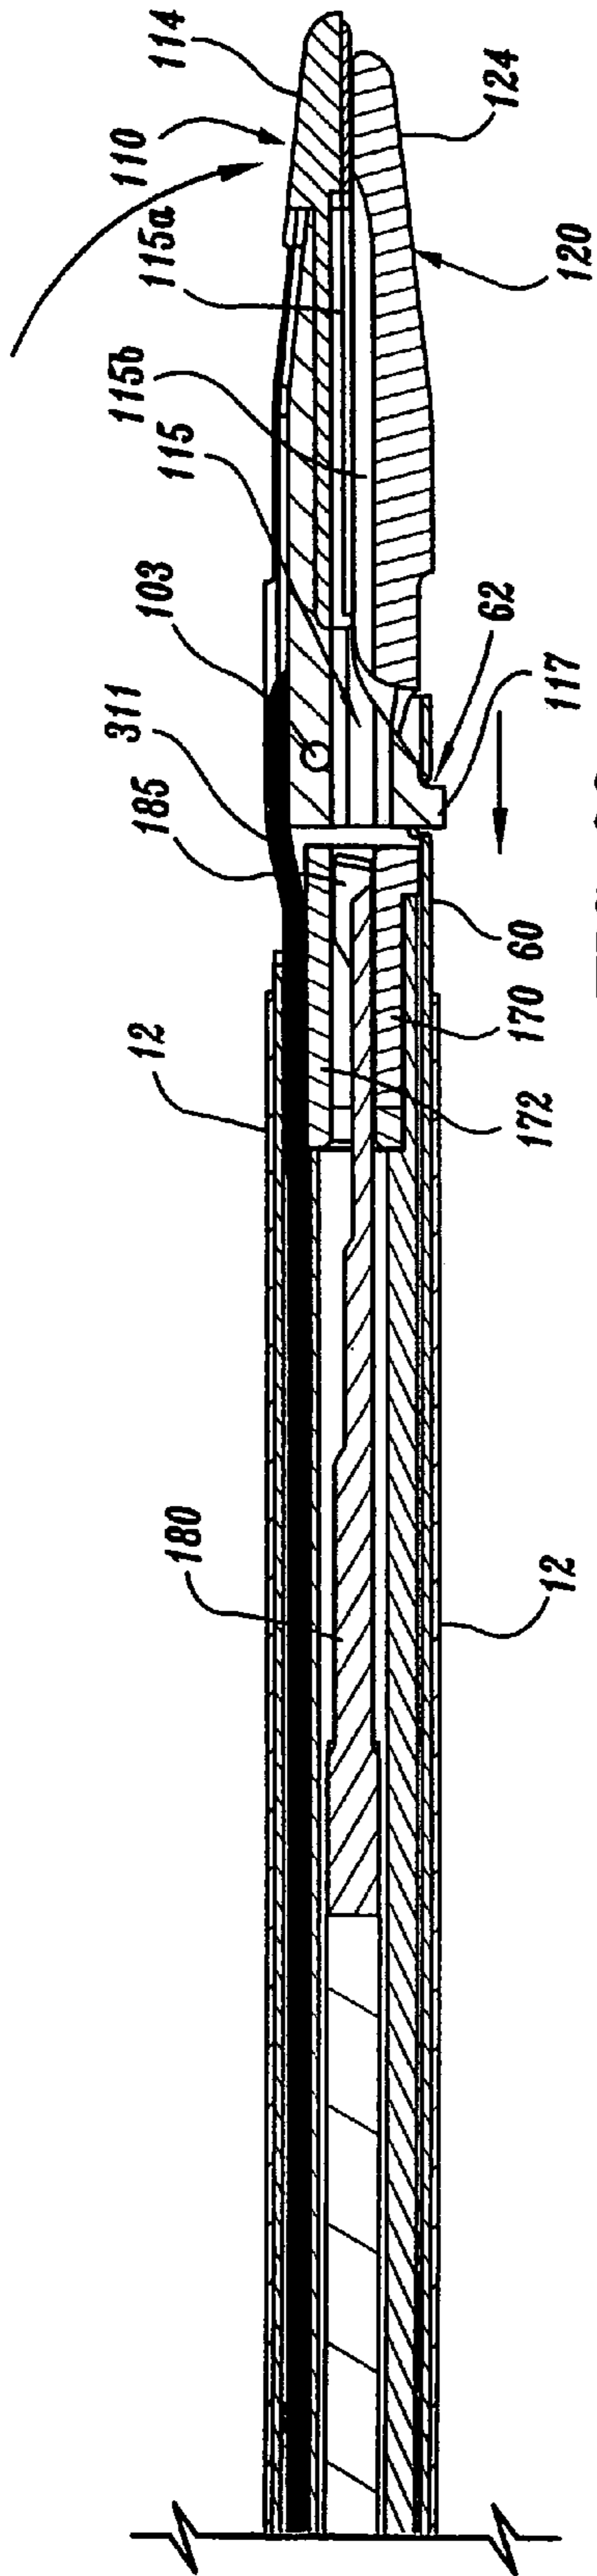


FIG. 39

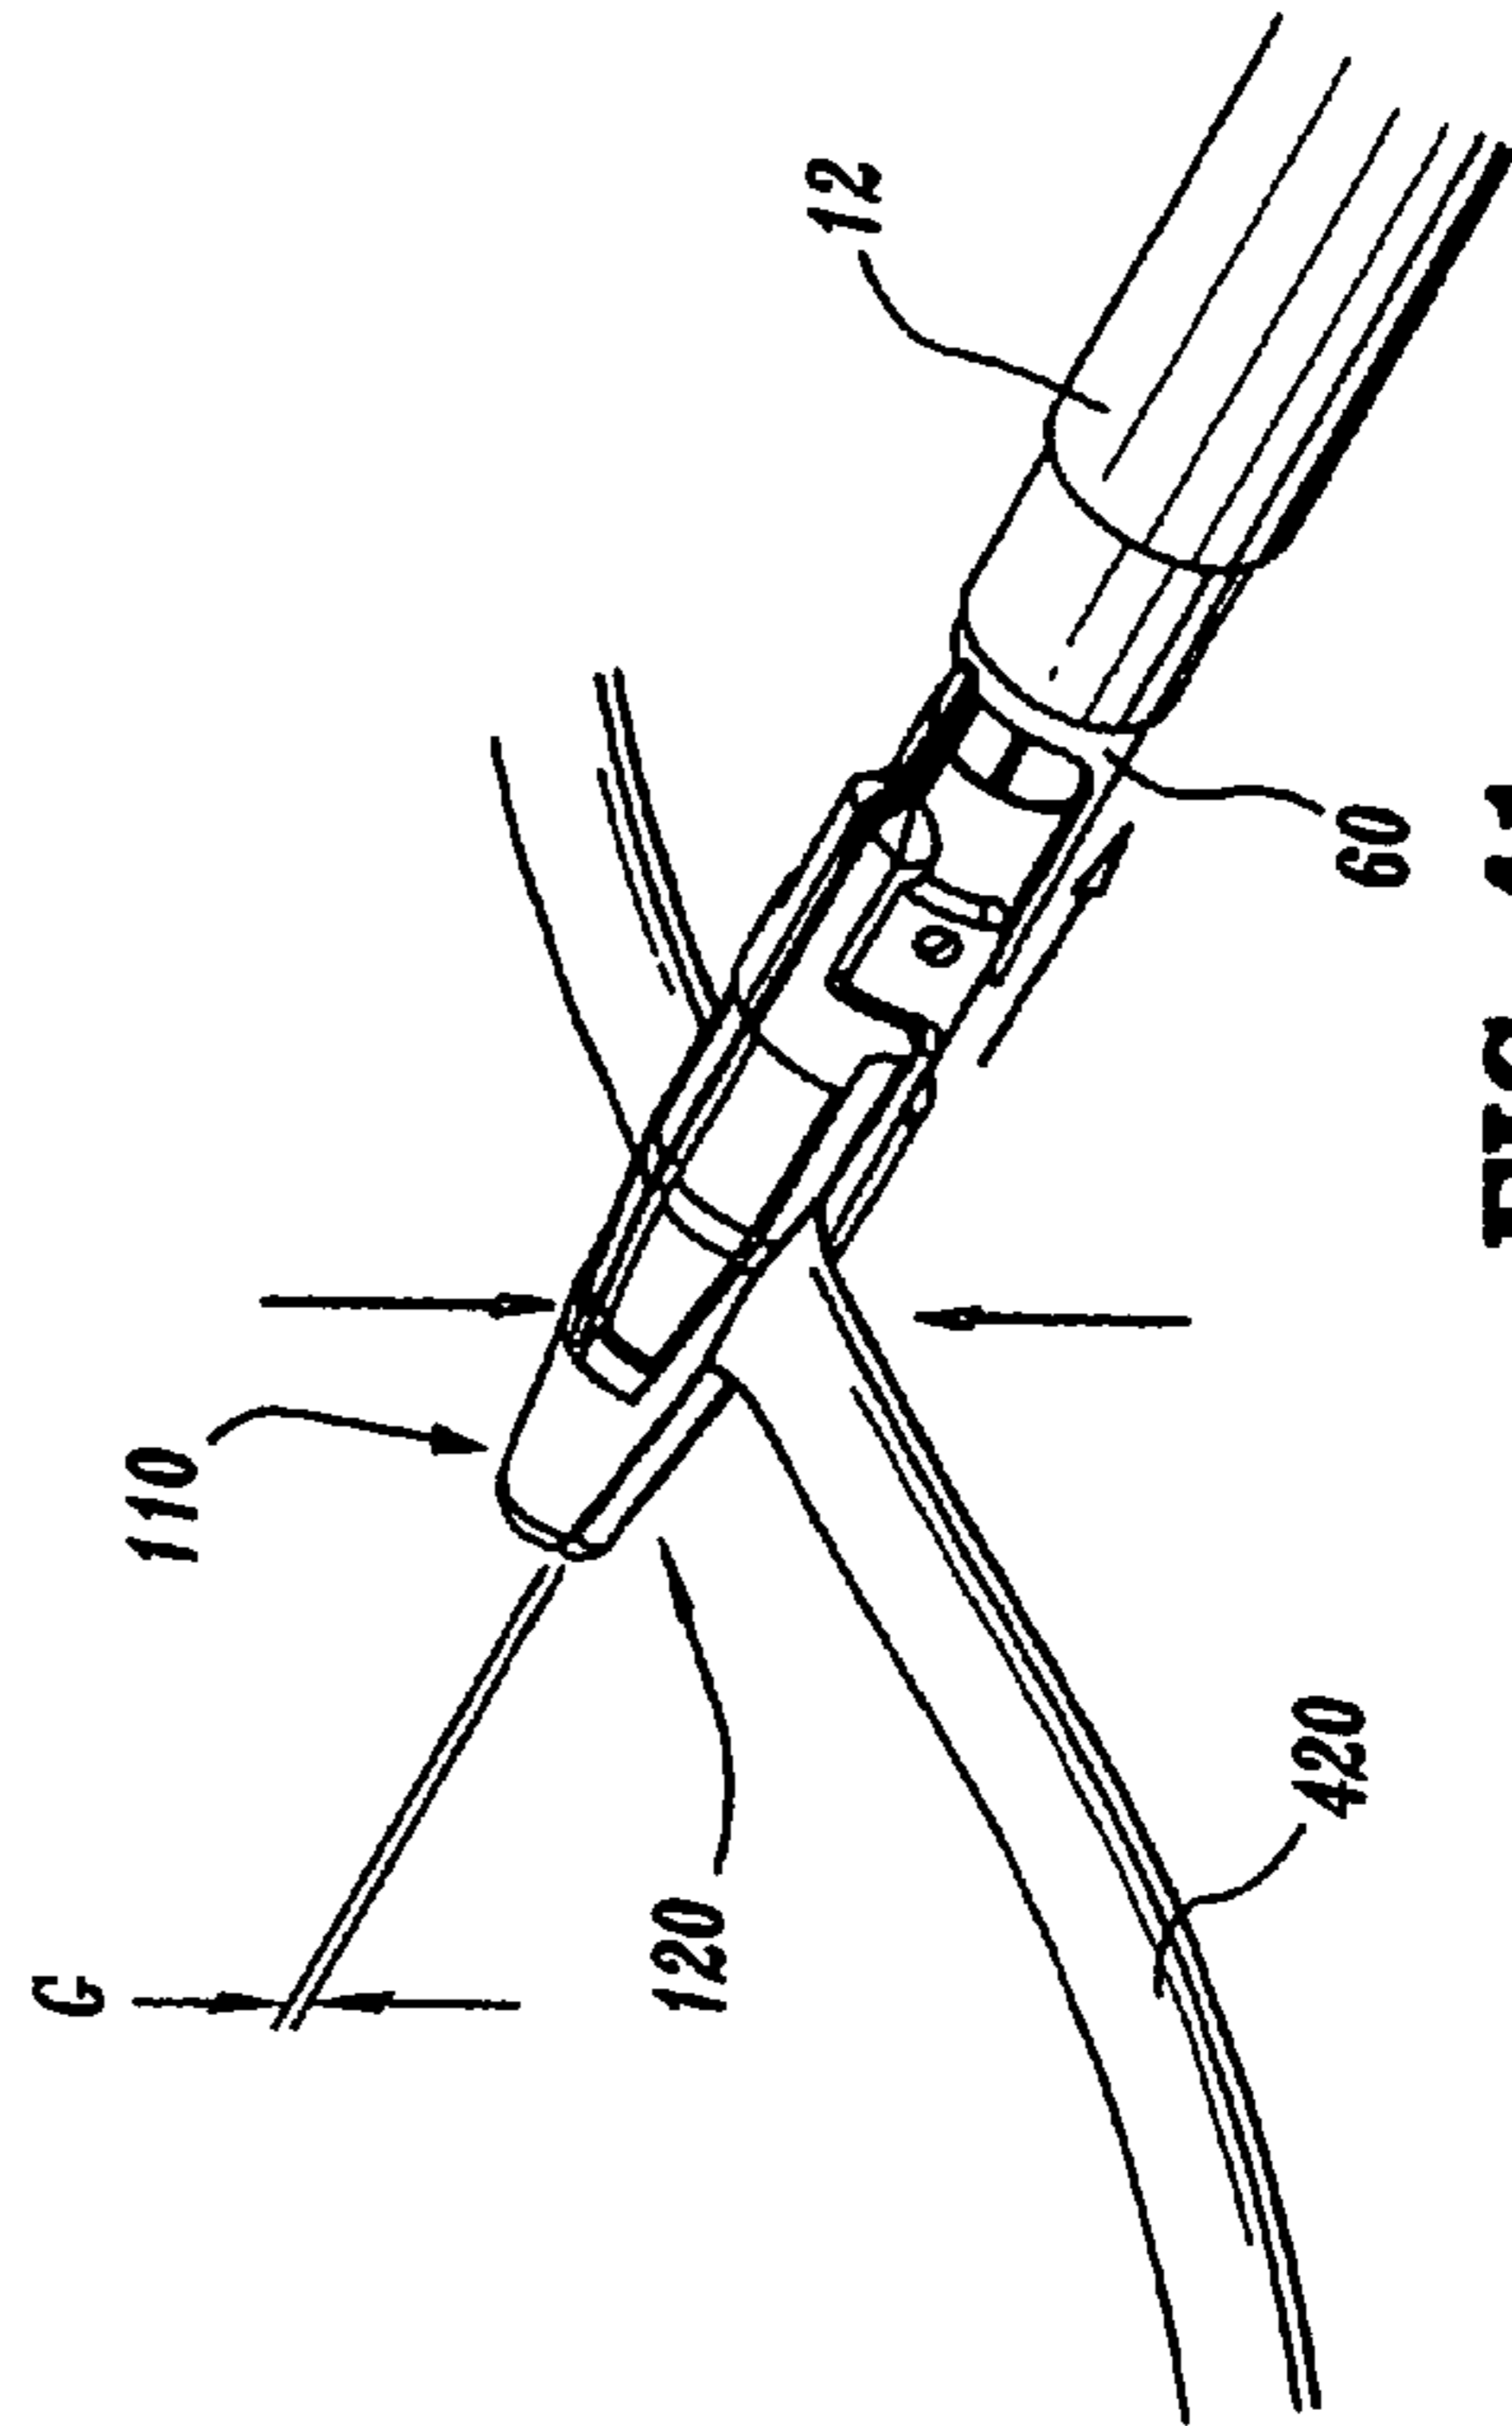


FIG. 41

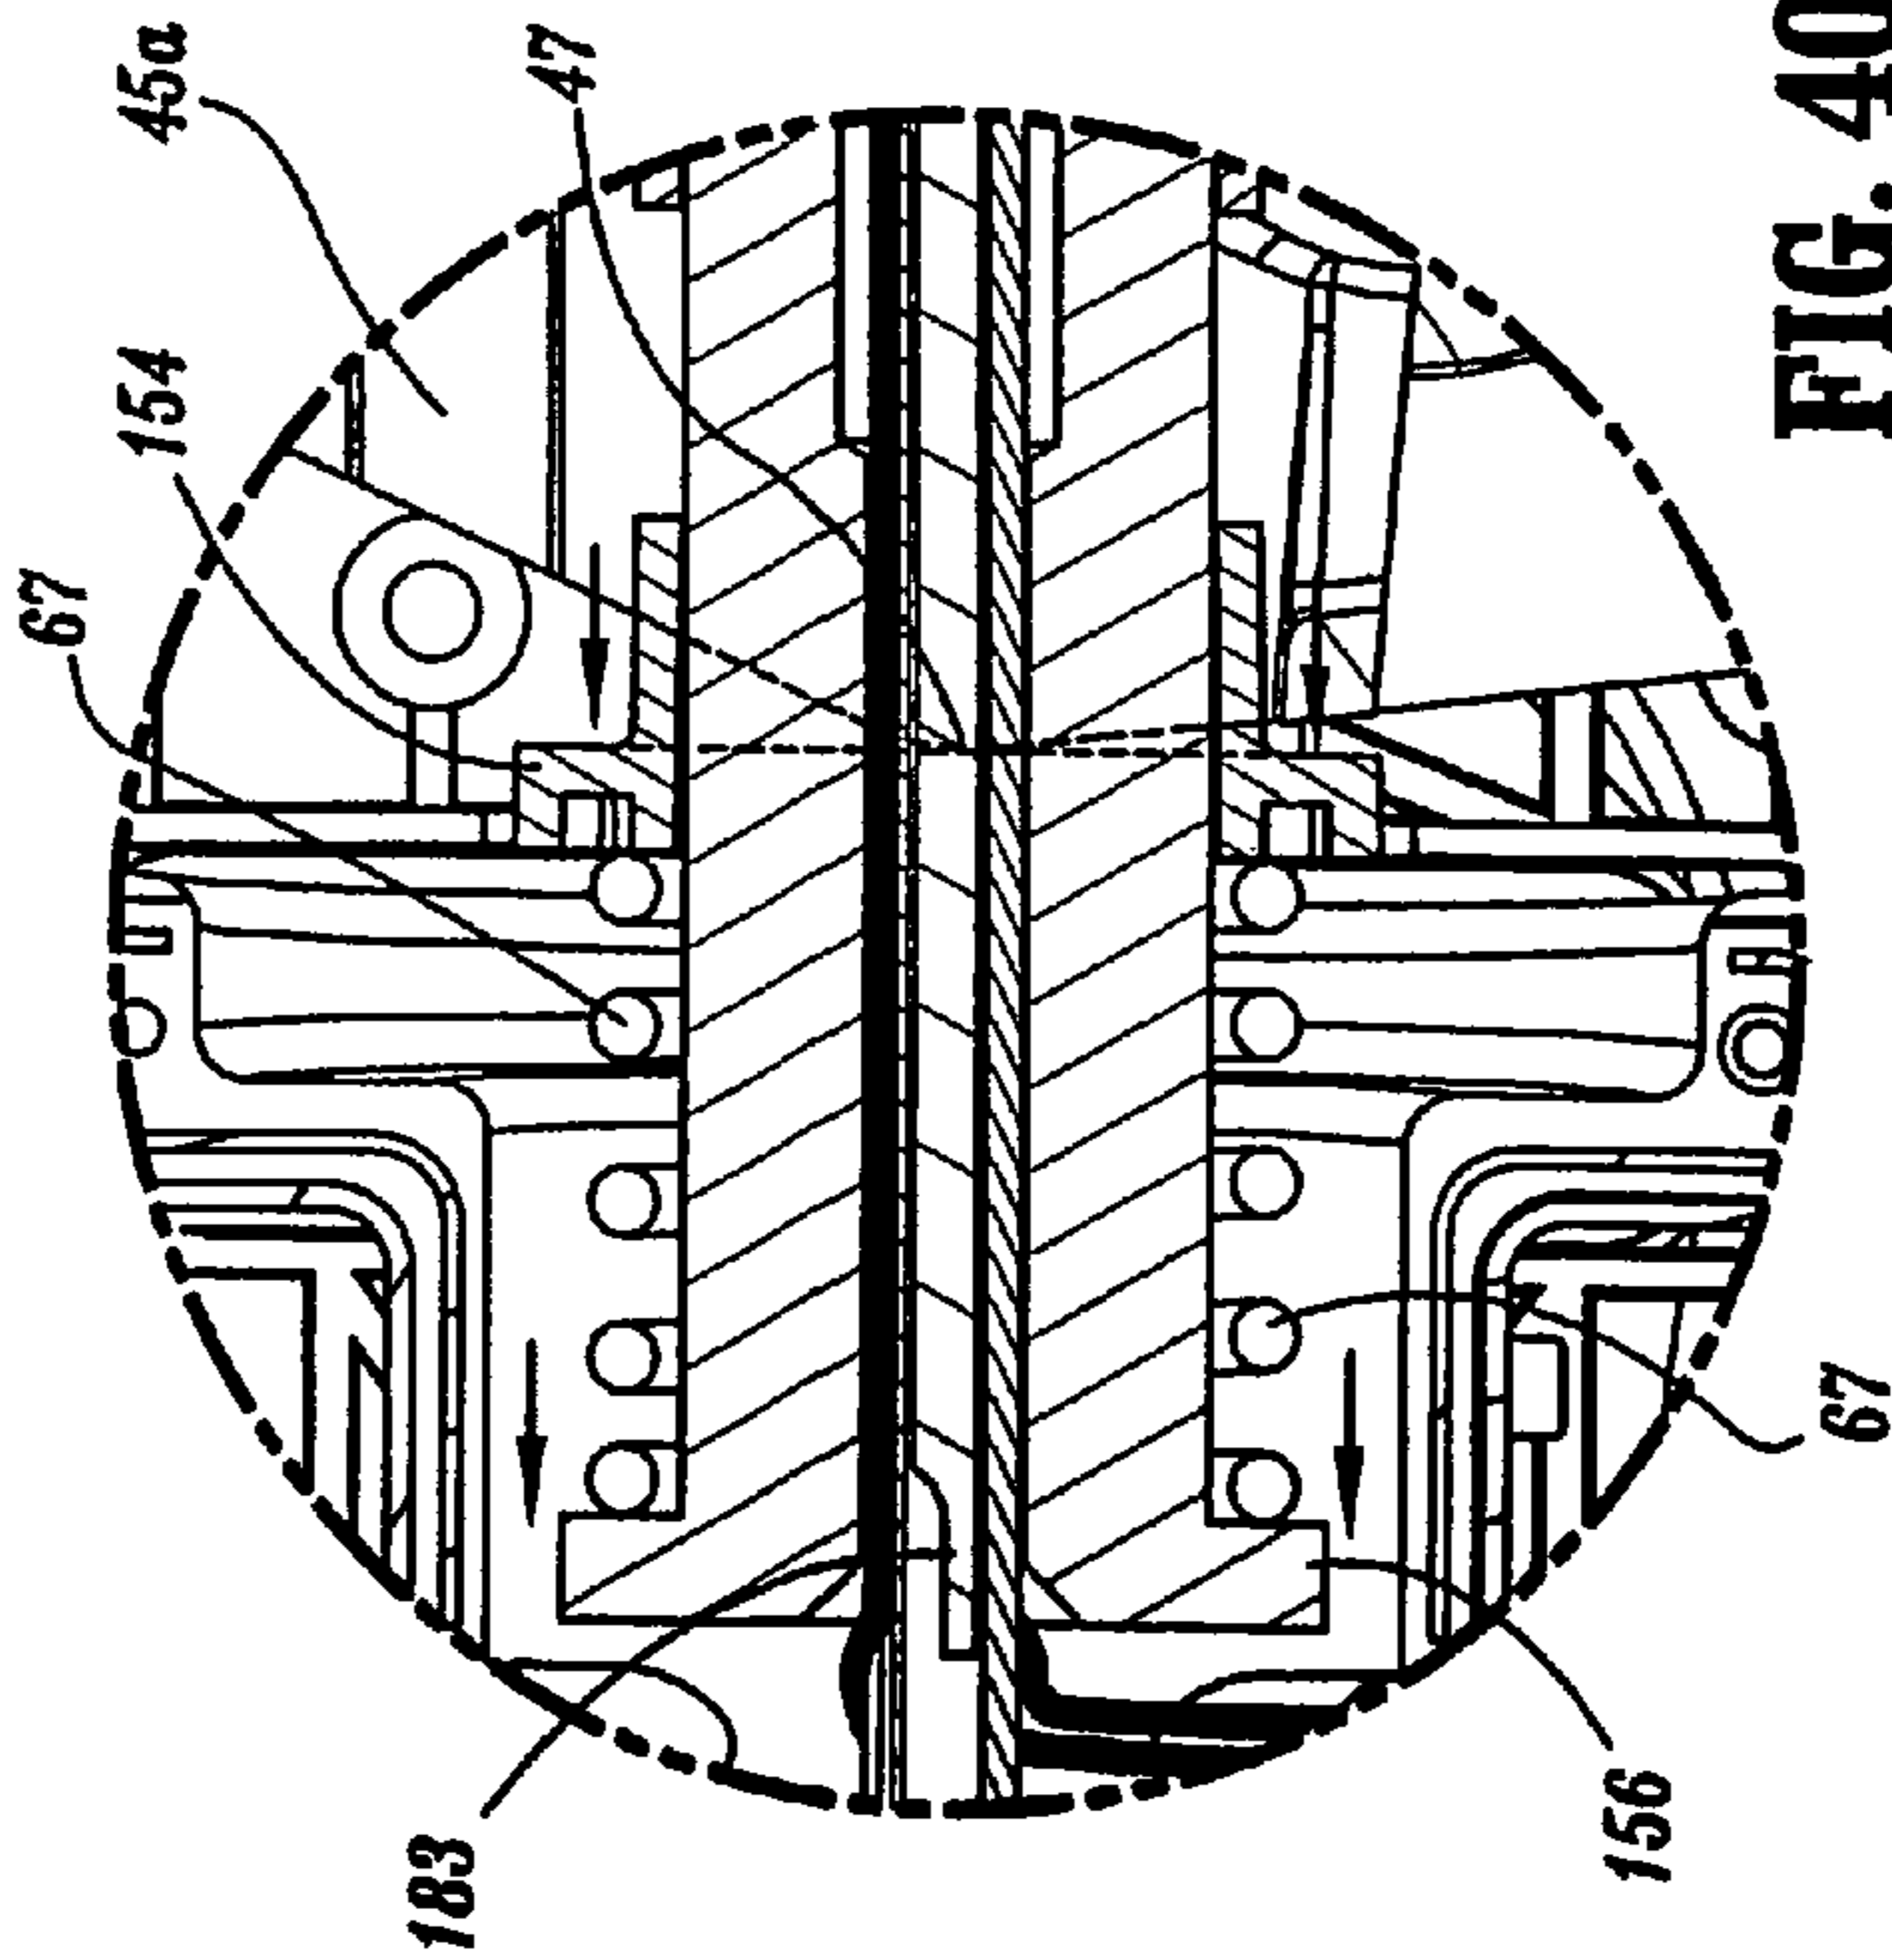


FIG. 40

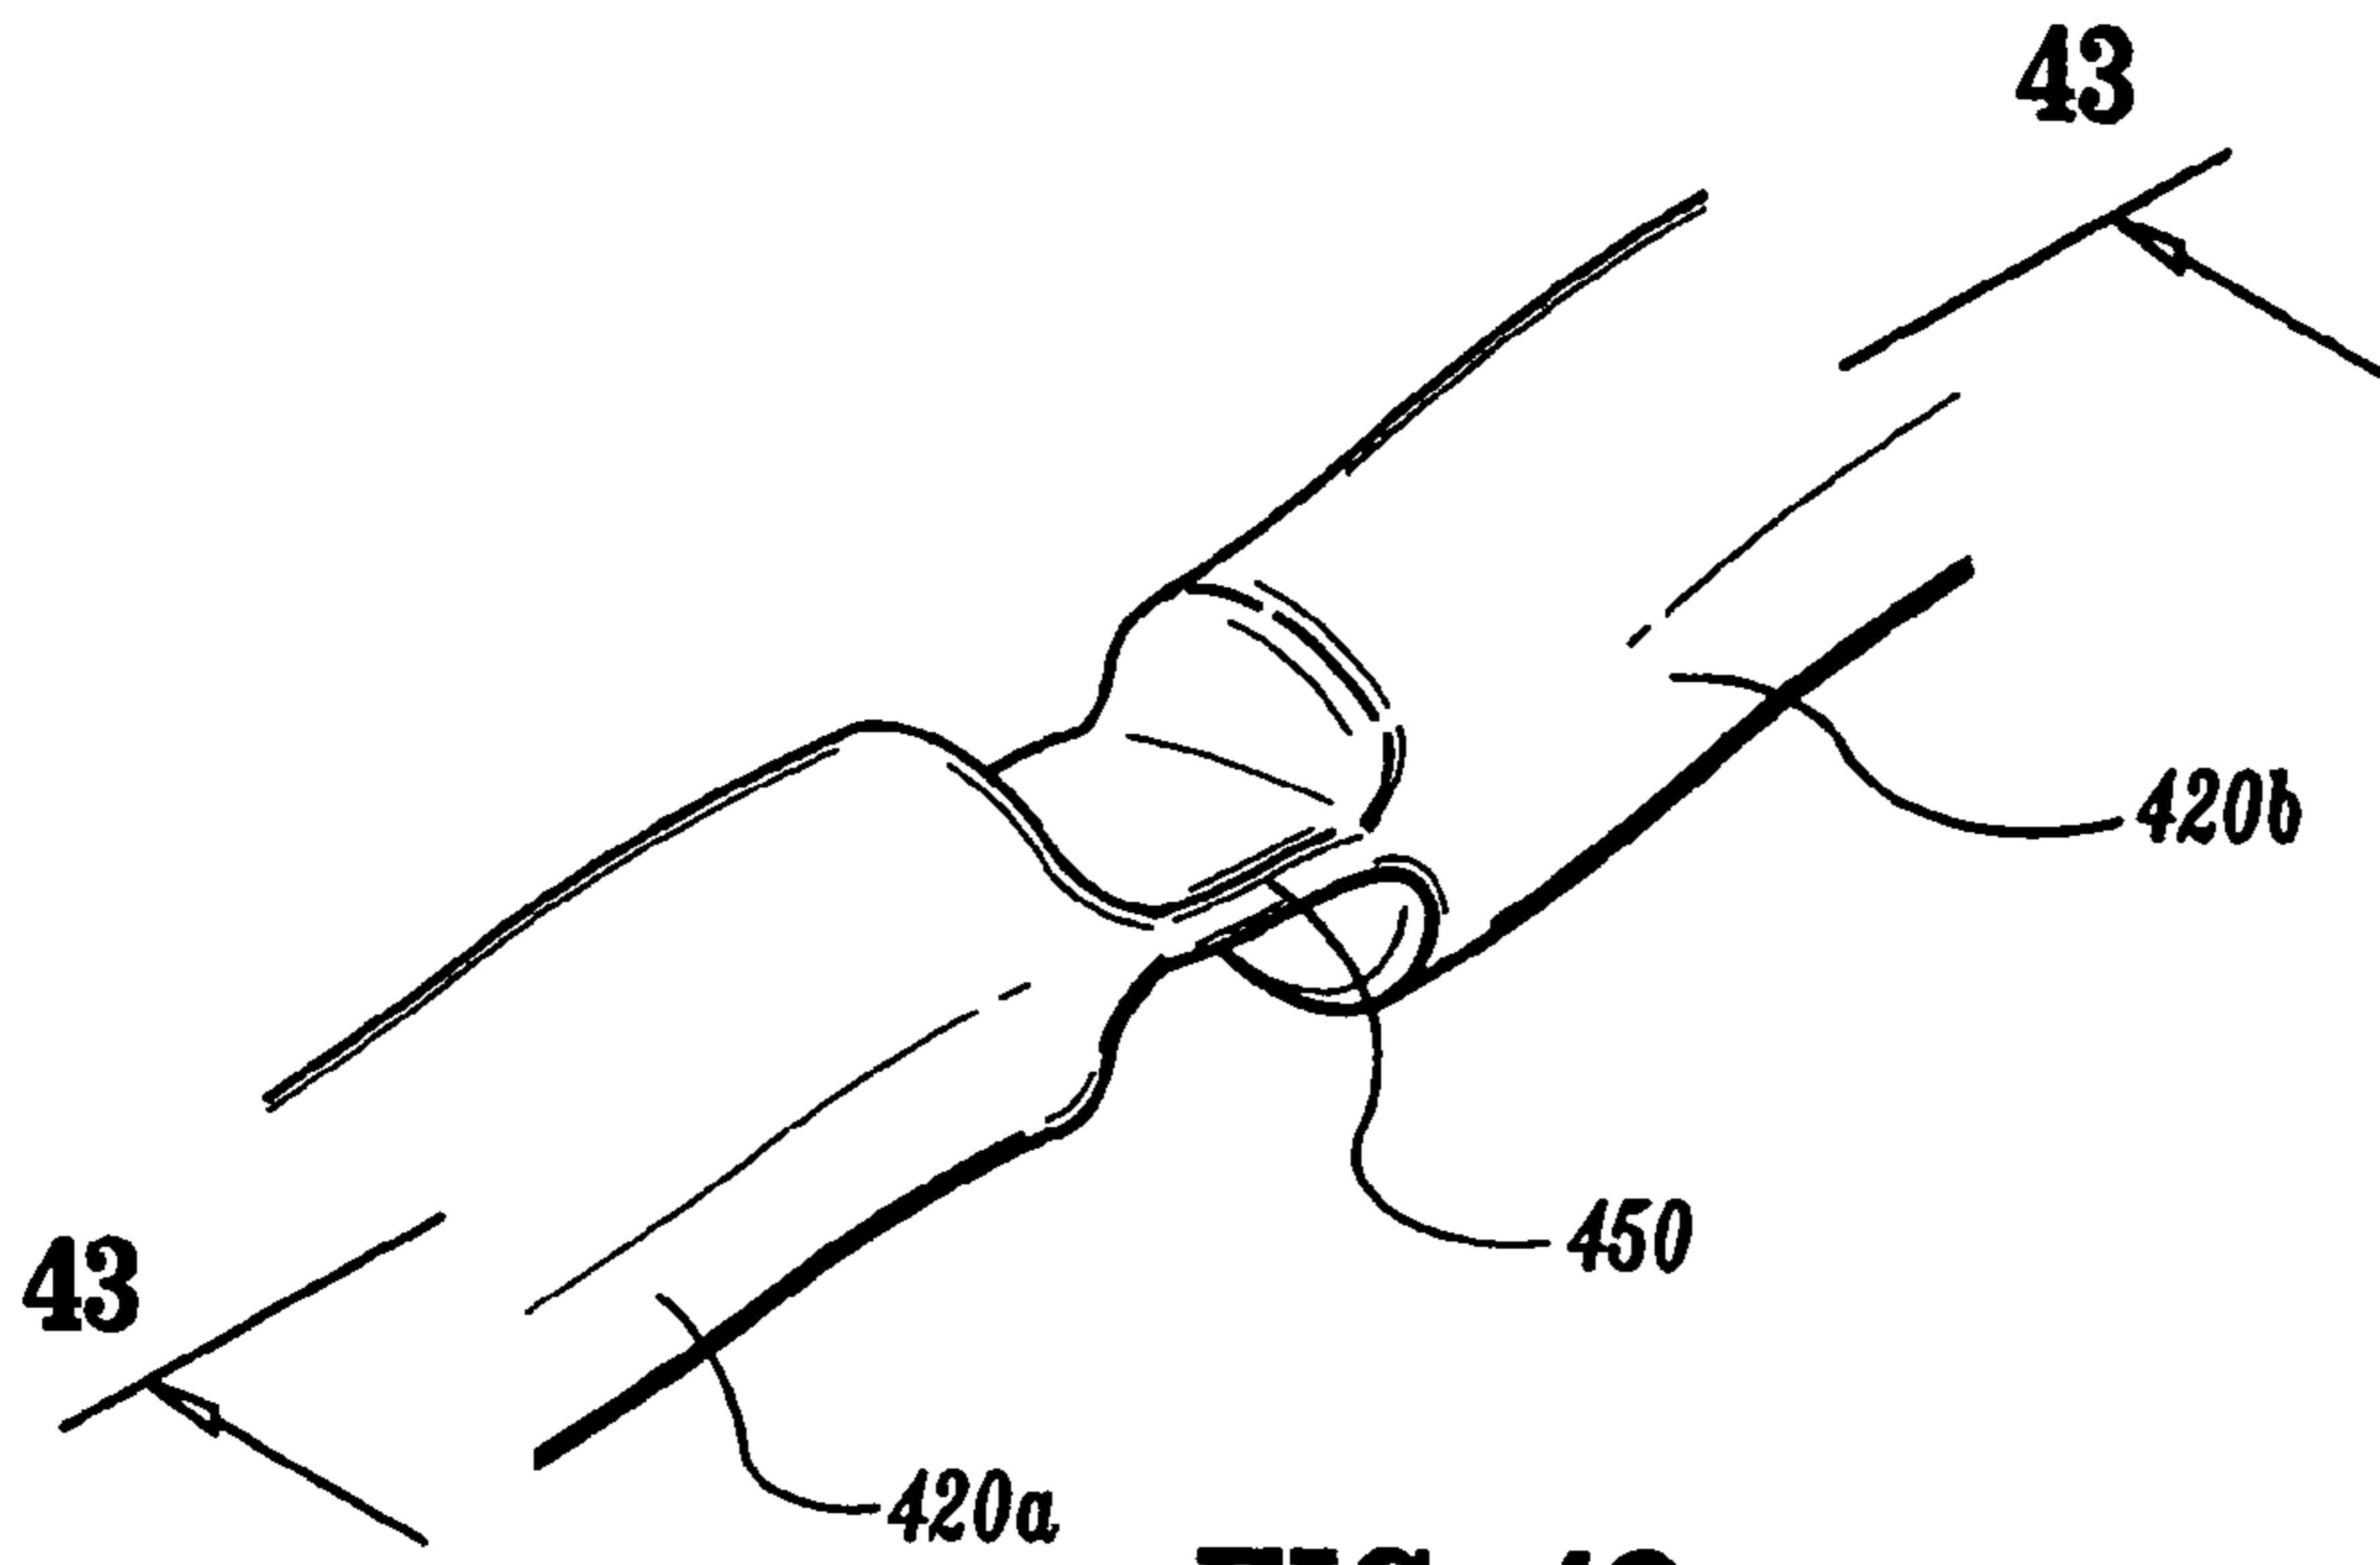


FIG. 42

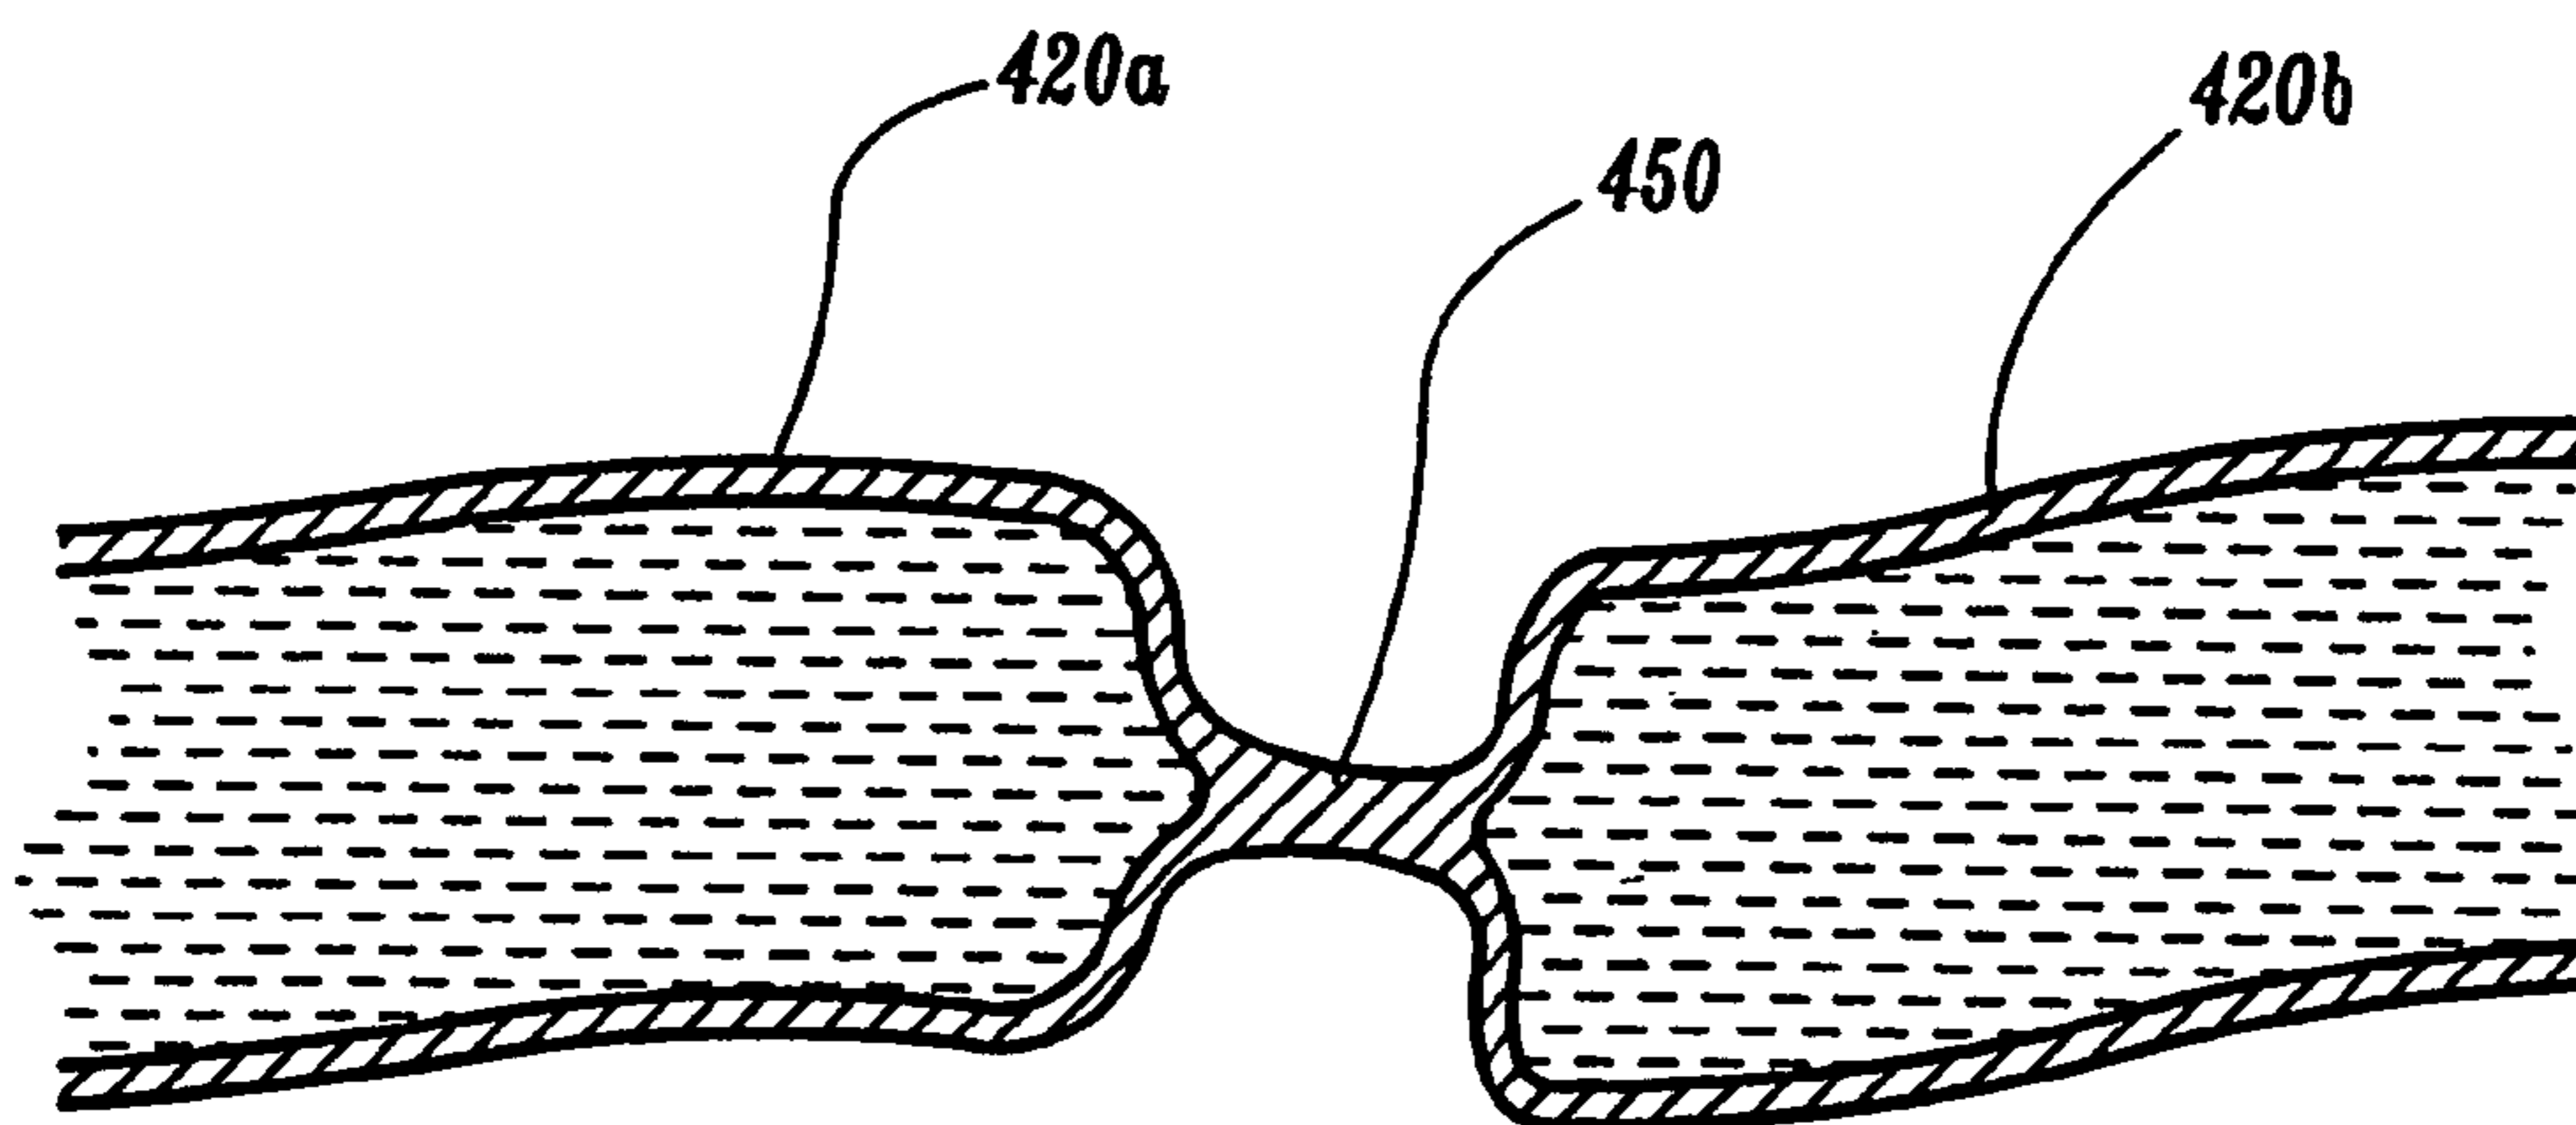


FIG. 43

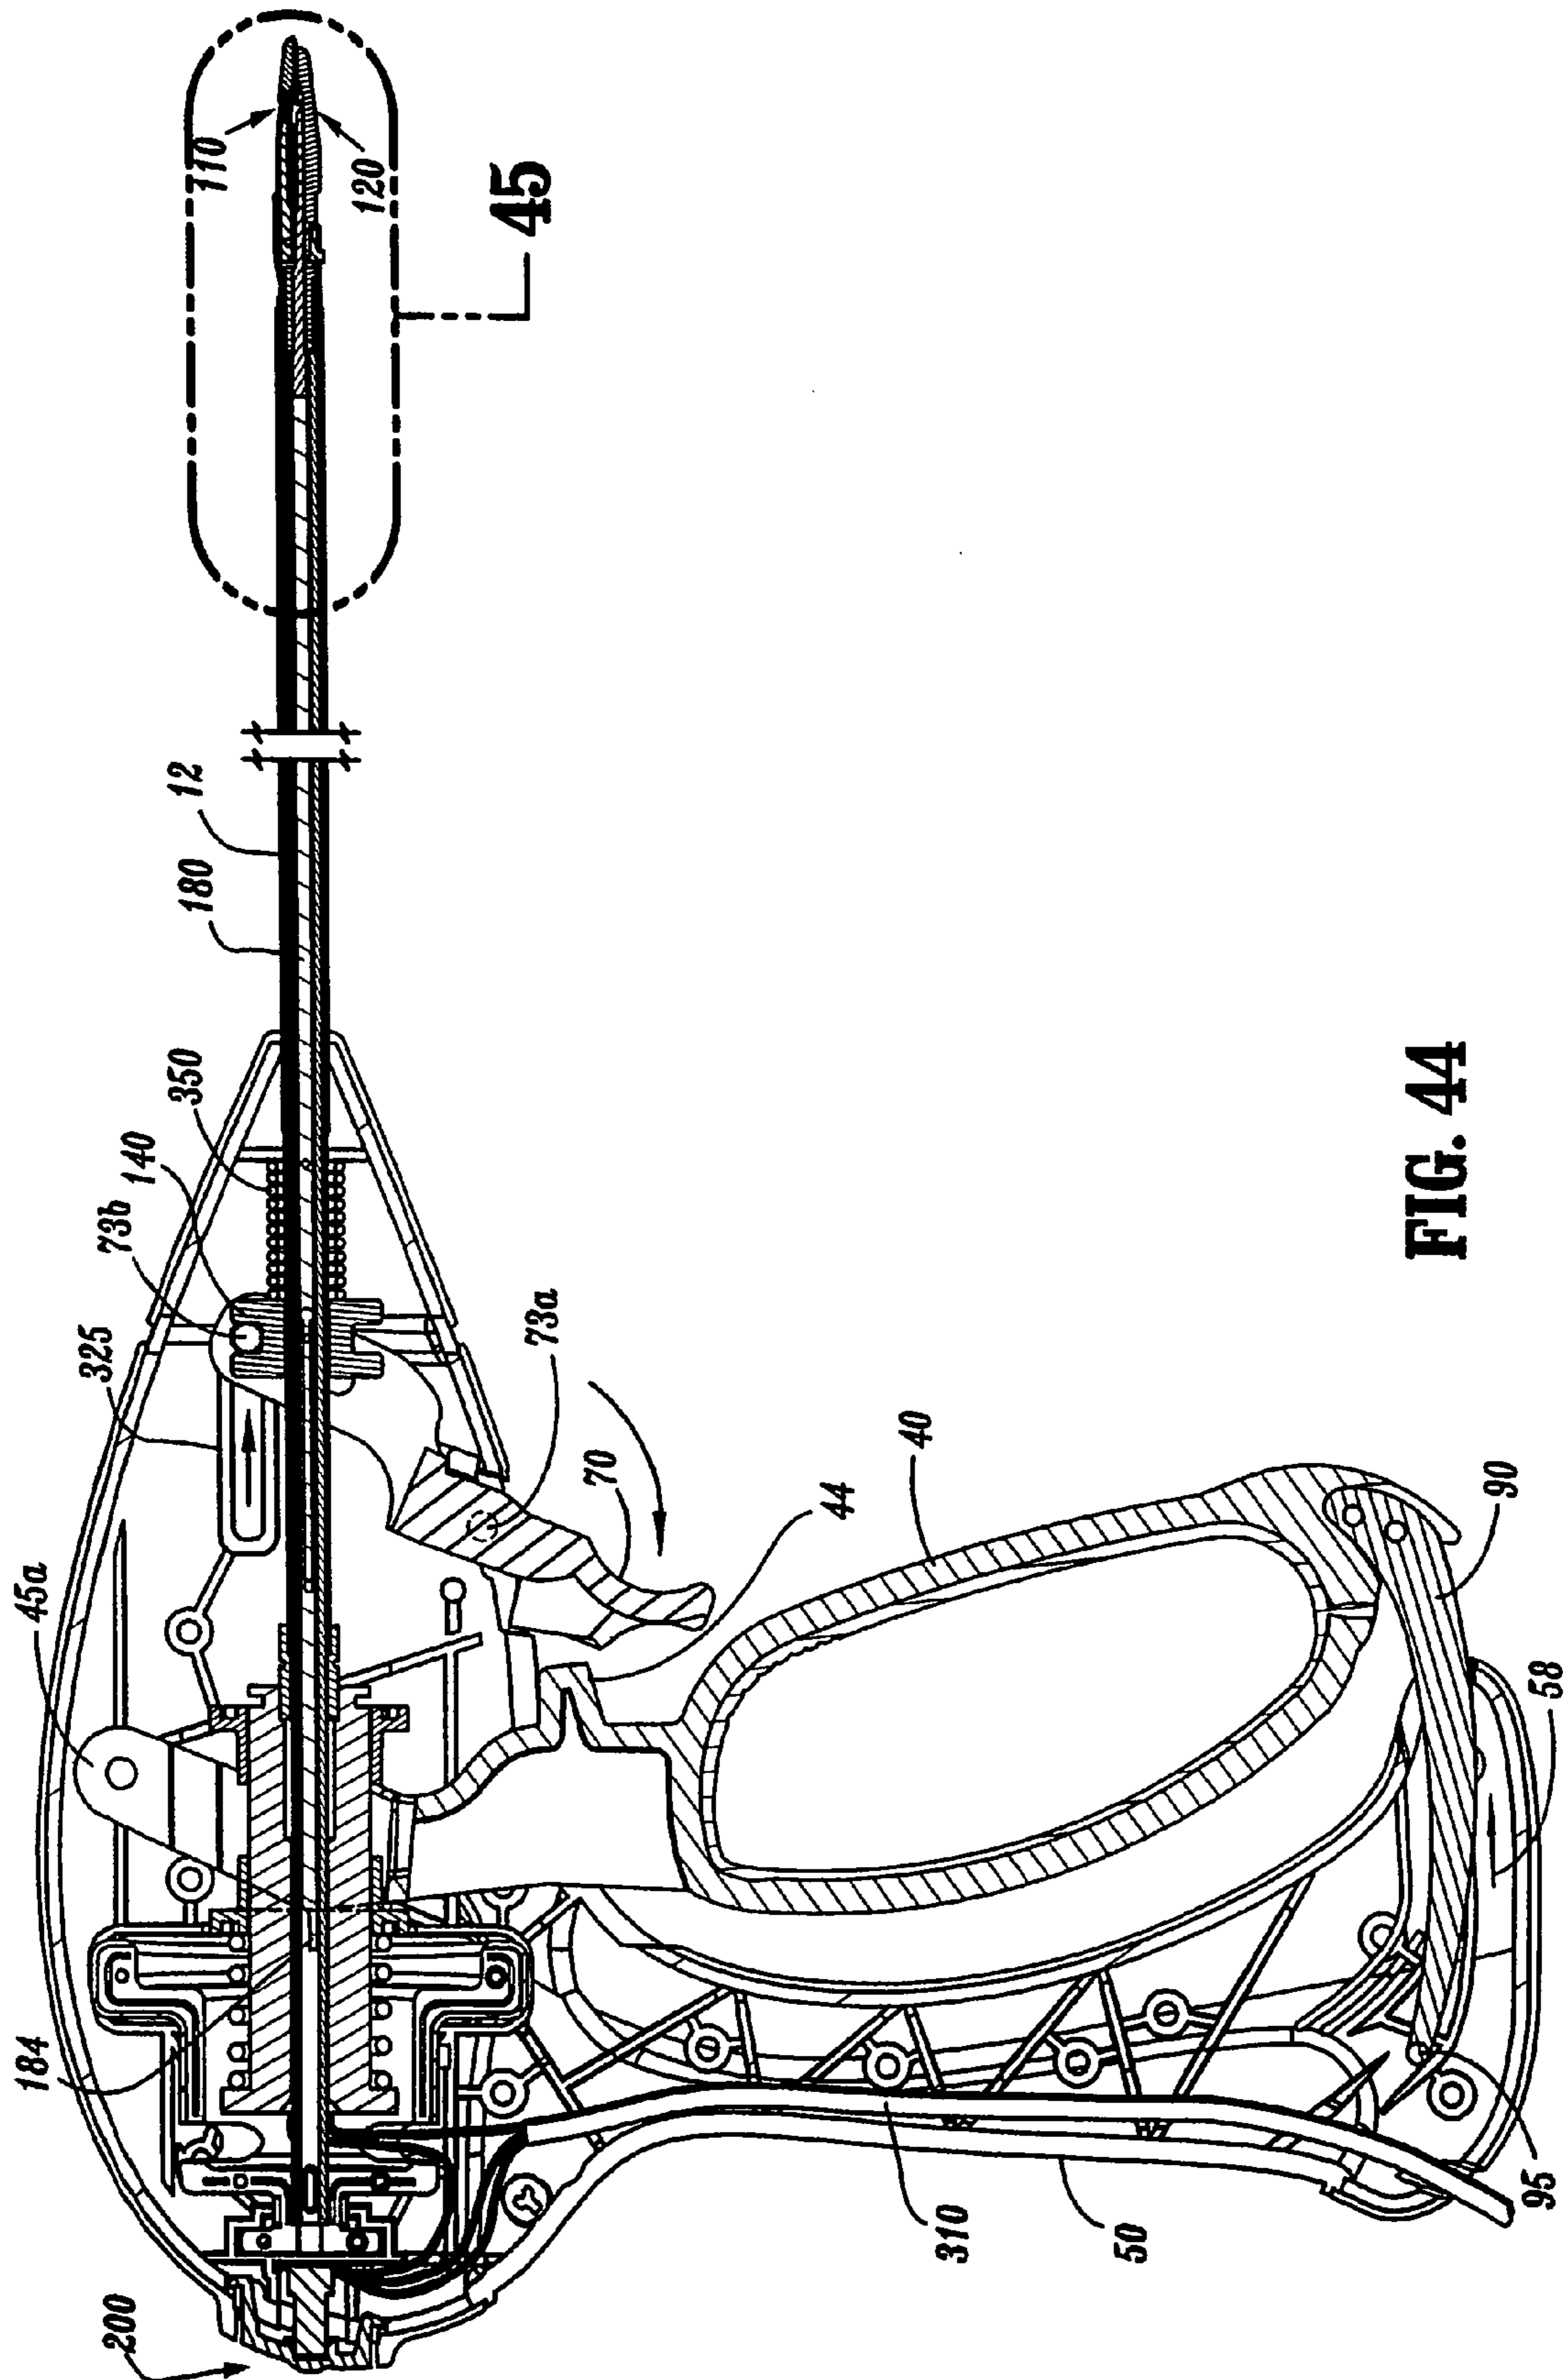


FIG. 44

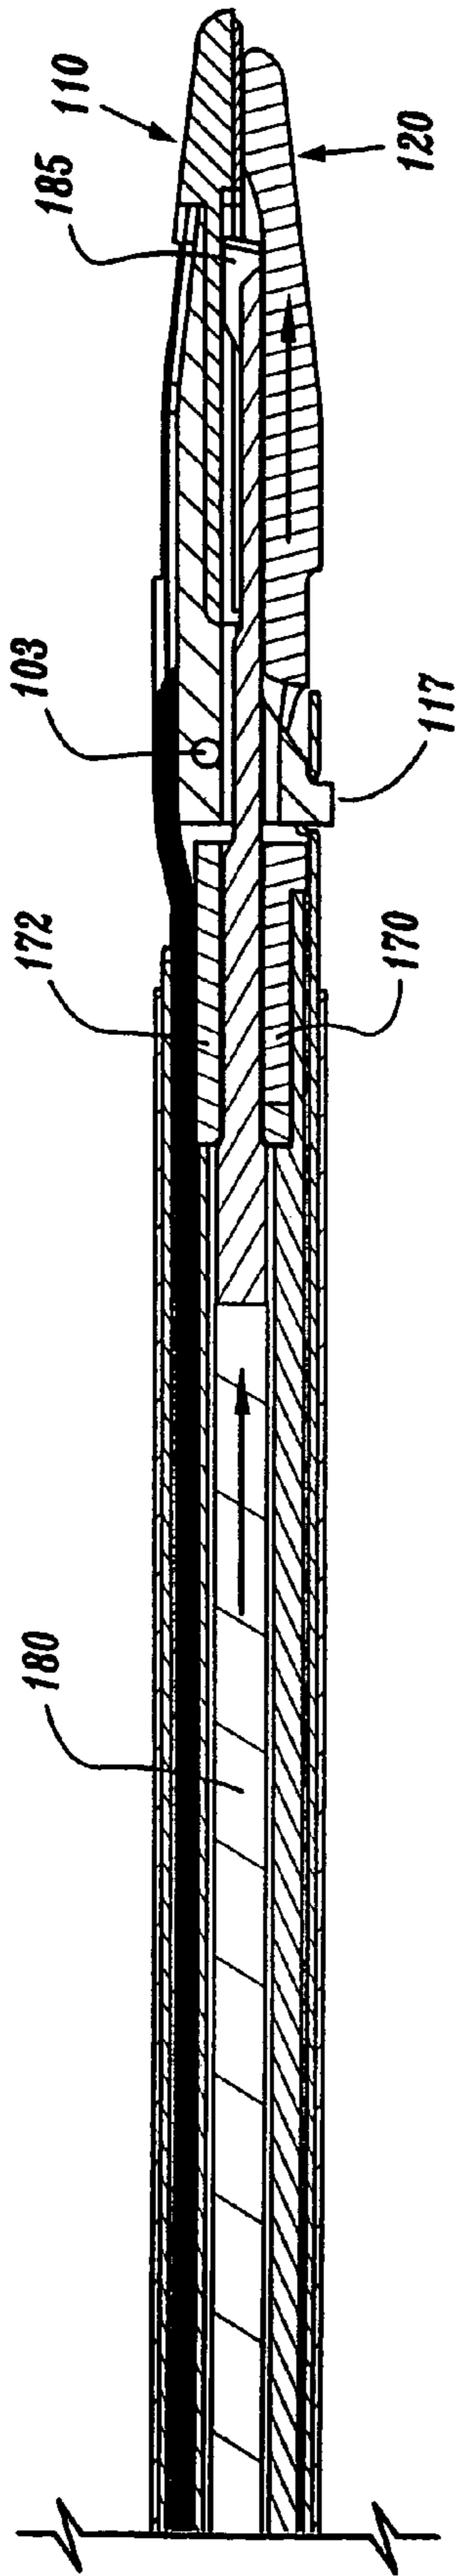


FIG. 45

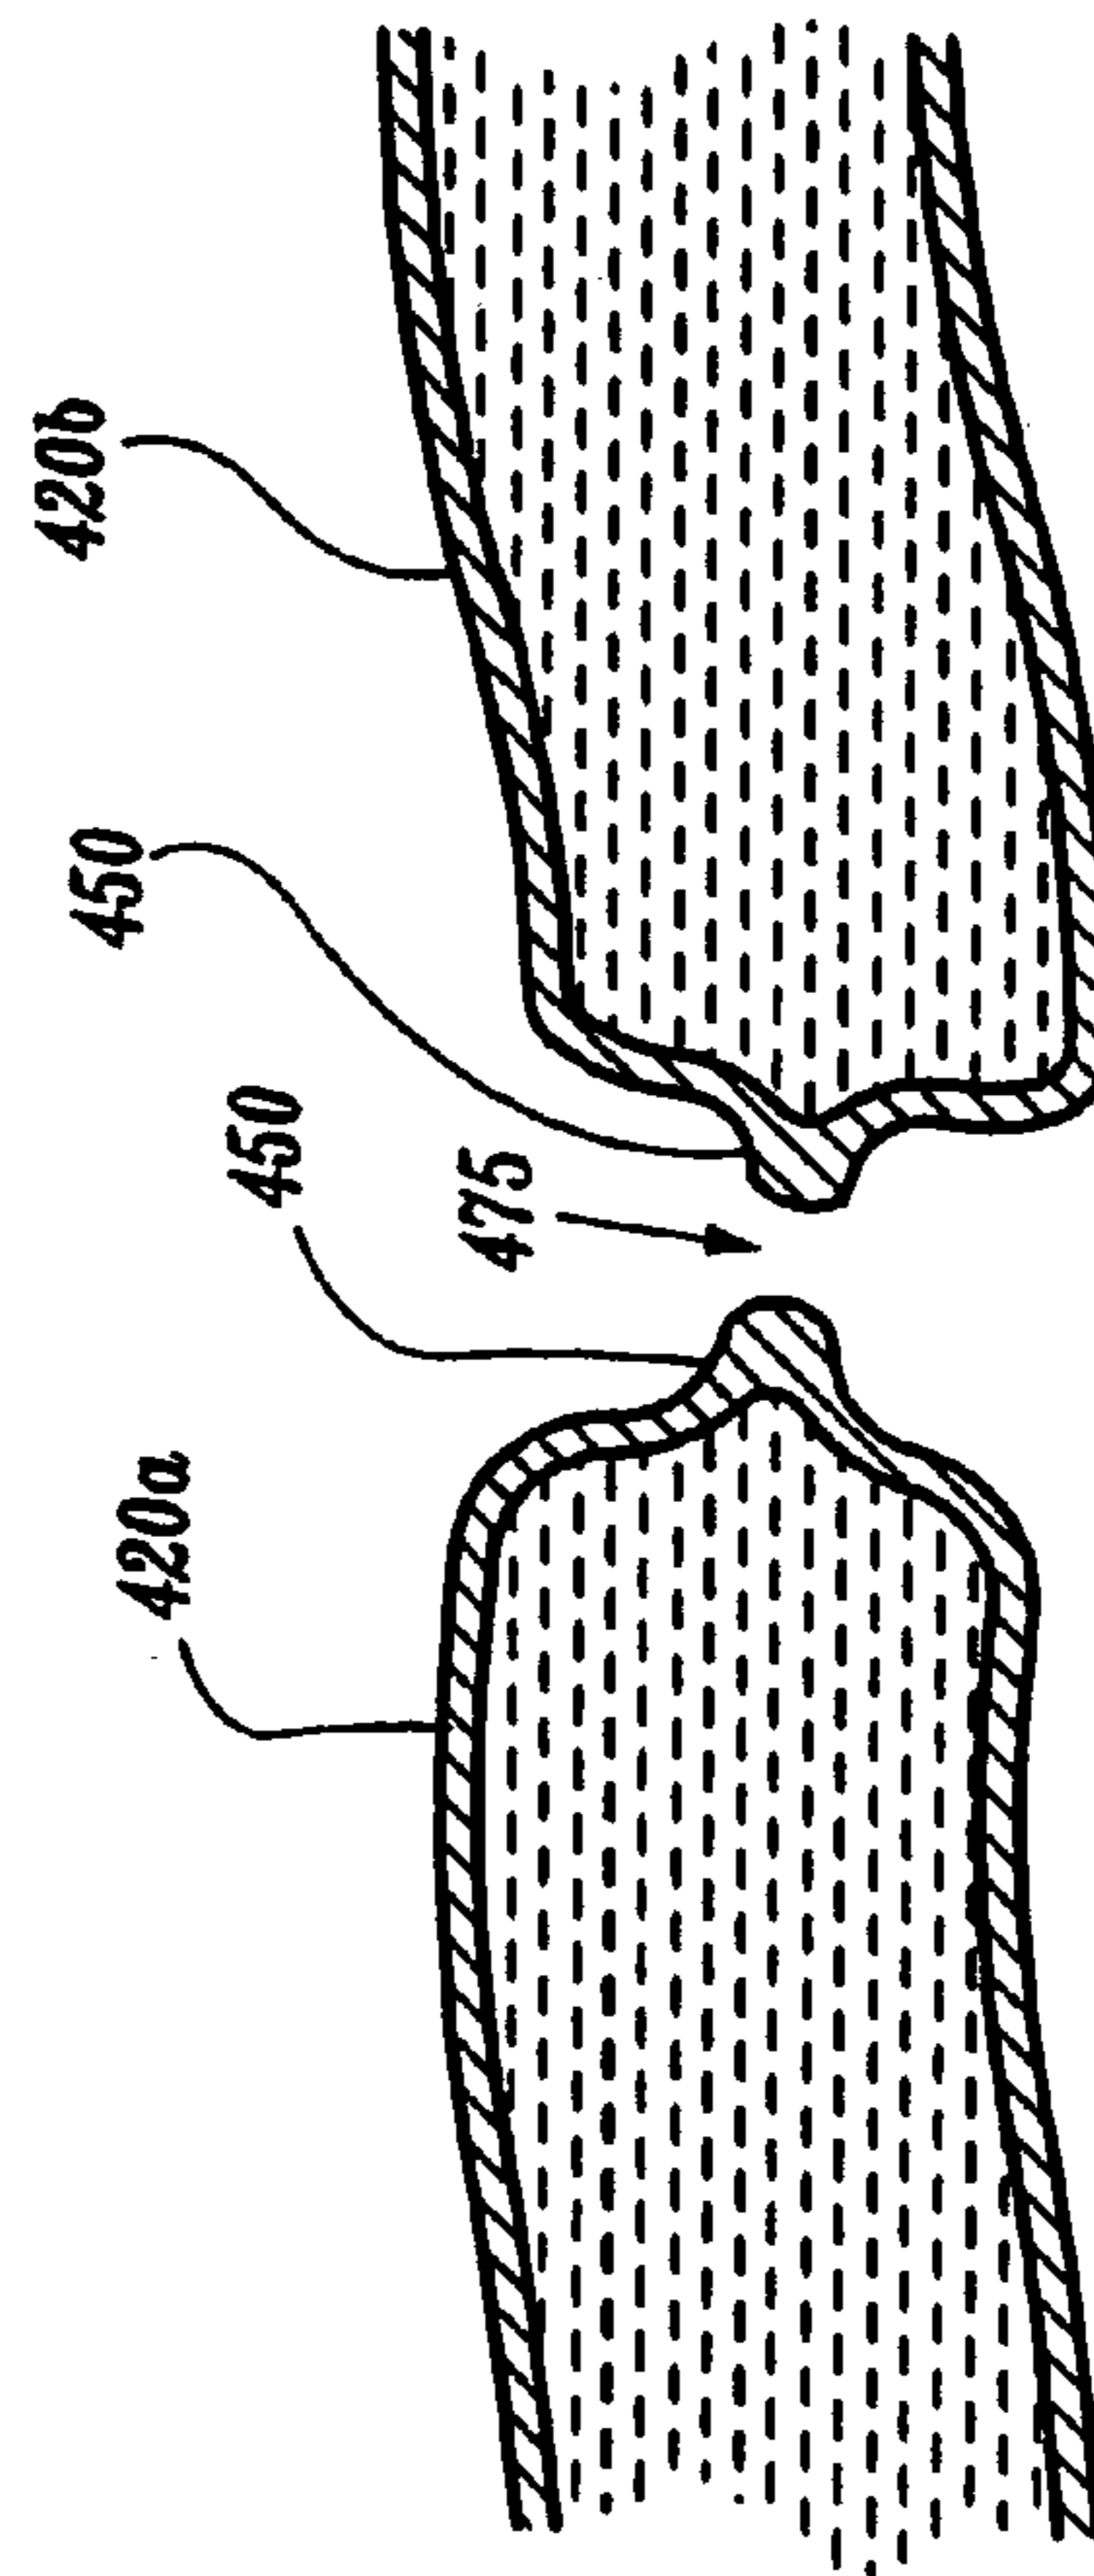


FIG. 46

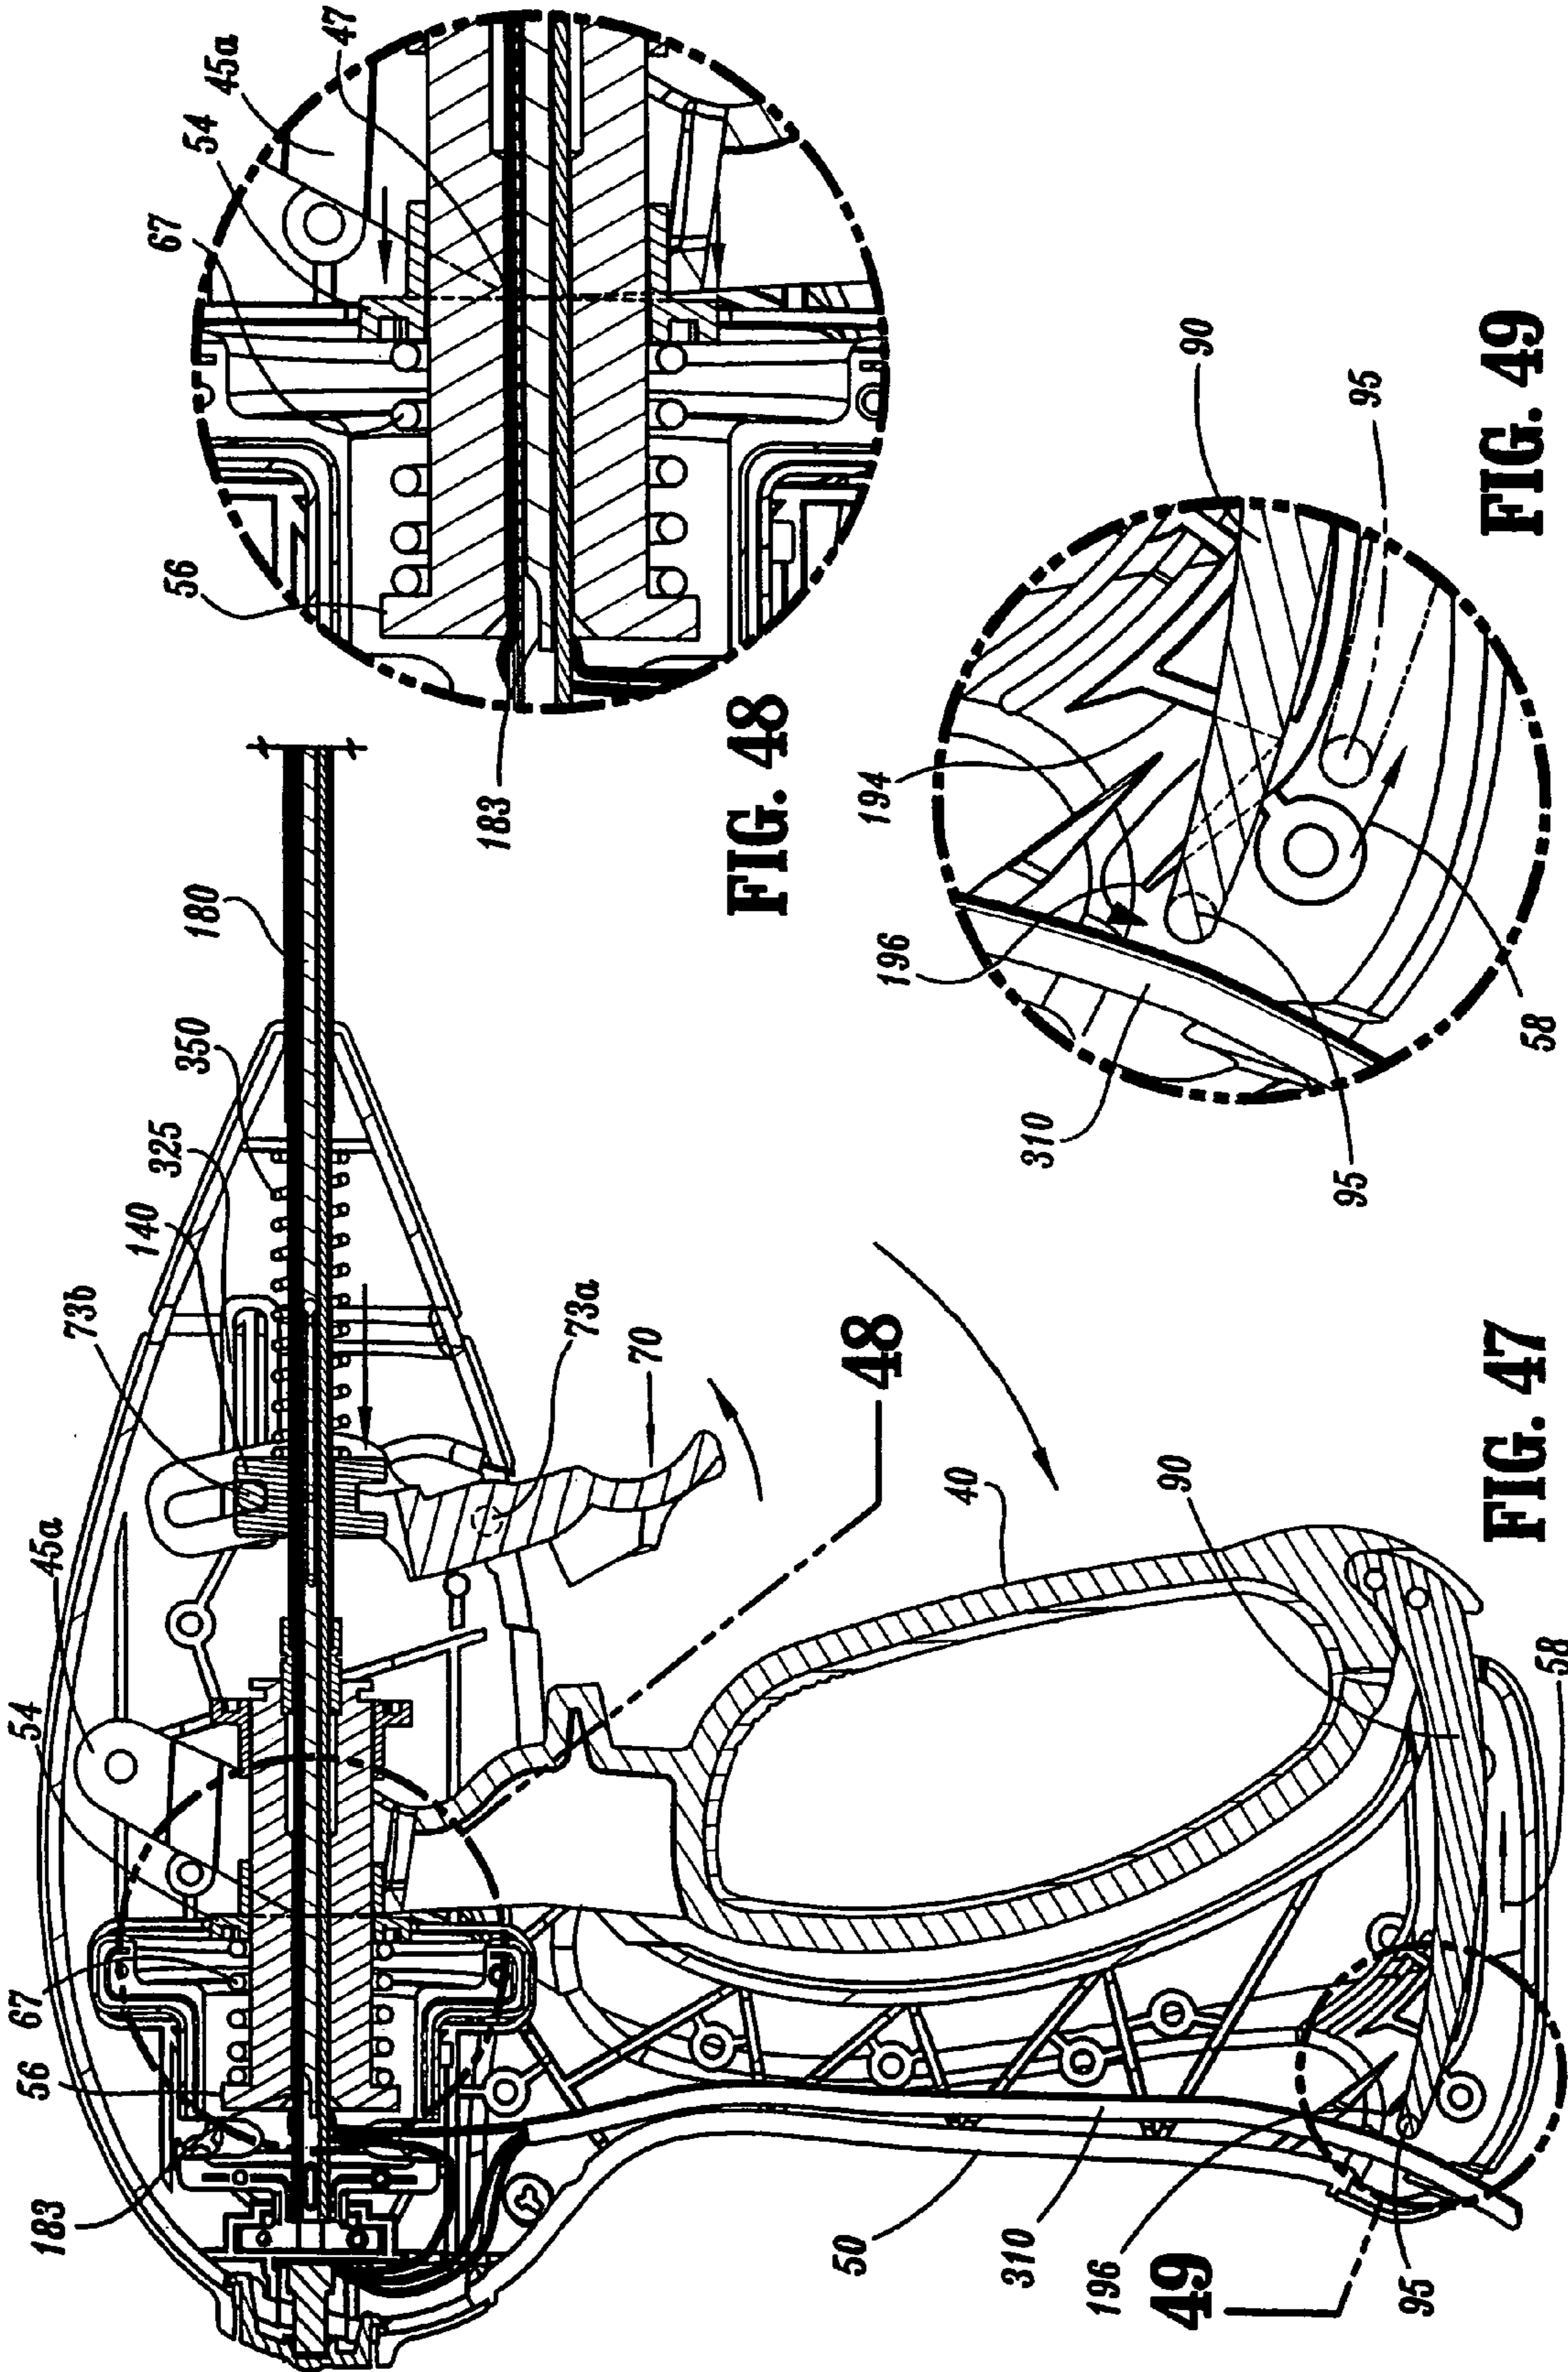


FIG. 48

FIG. 49

FIG. 47

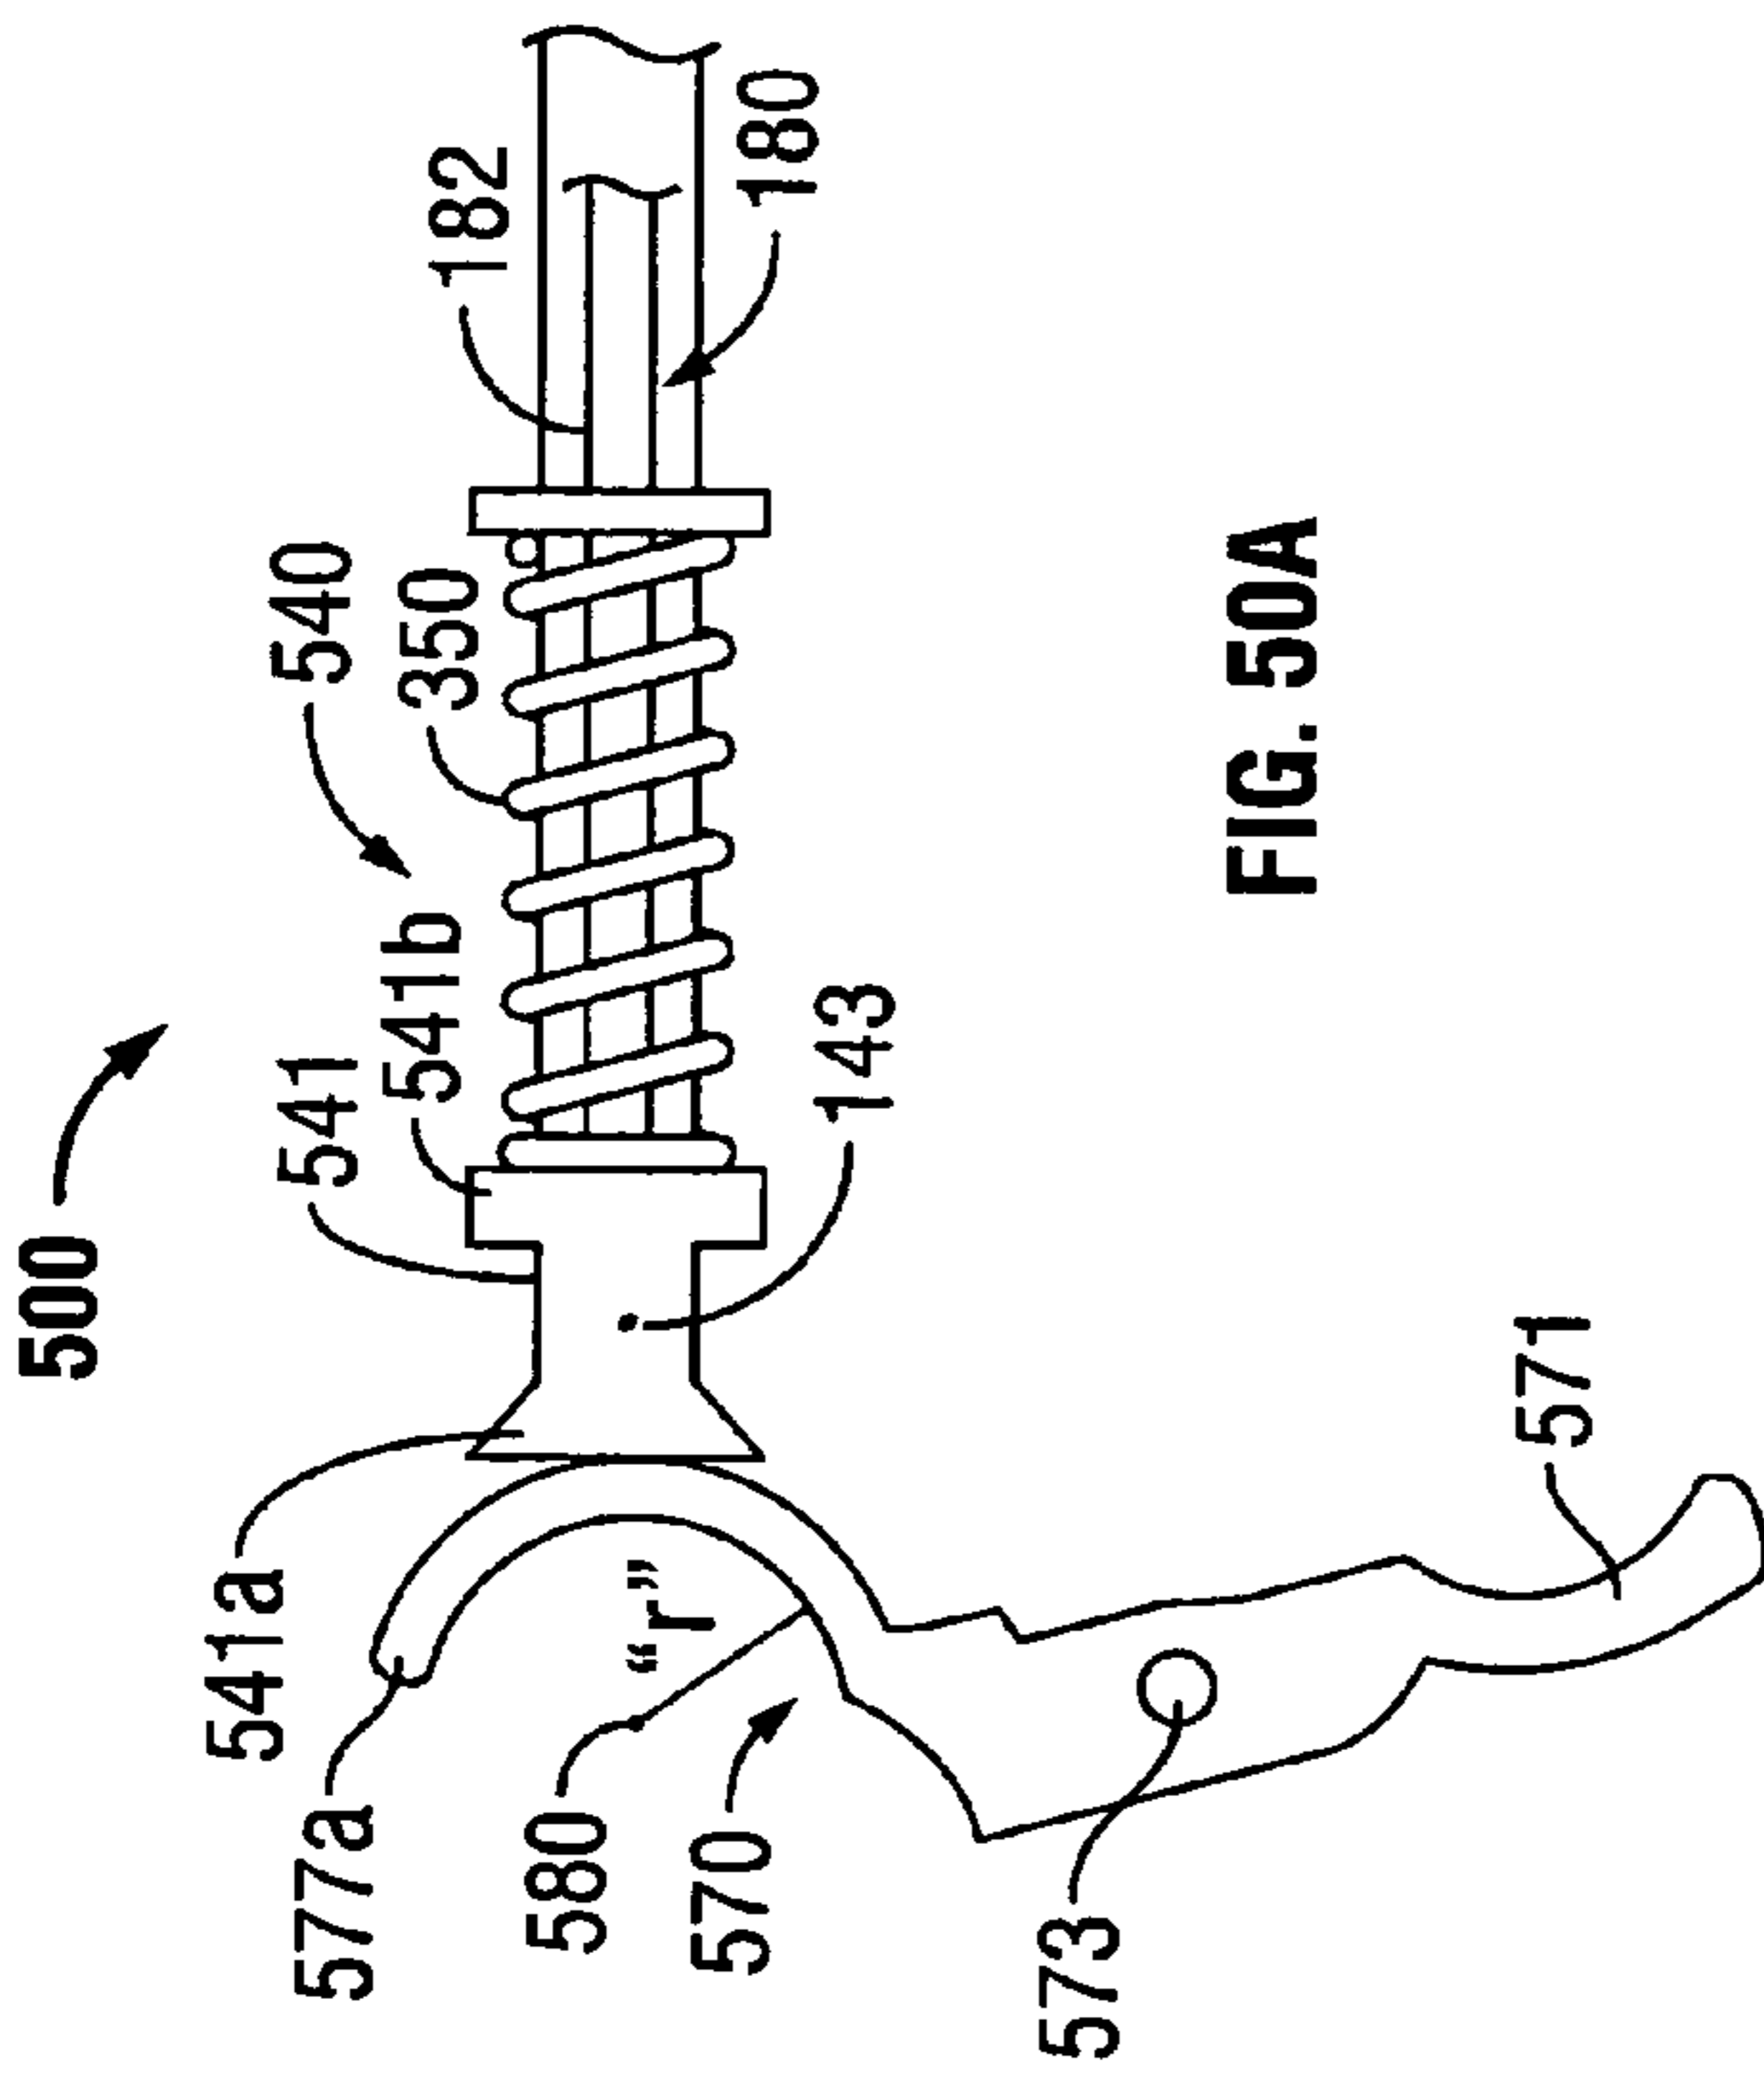


FIG. 50A

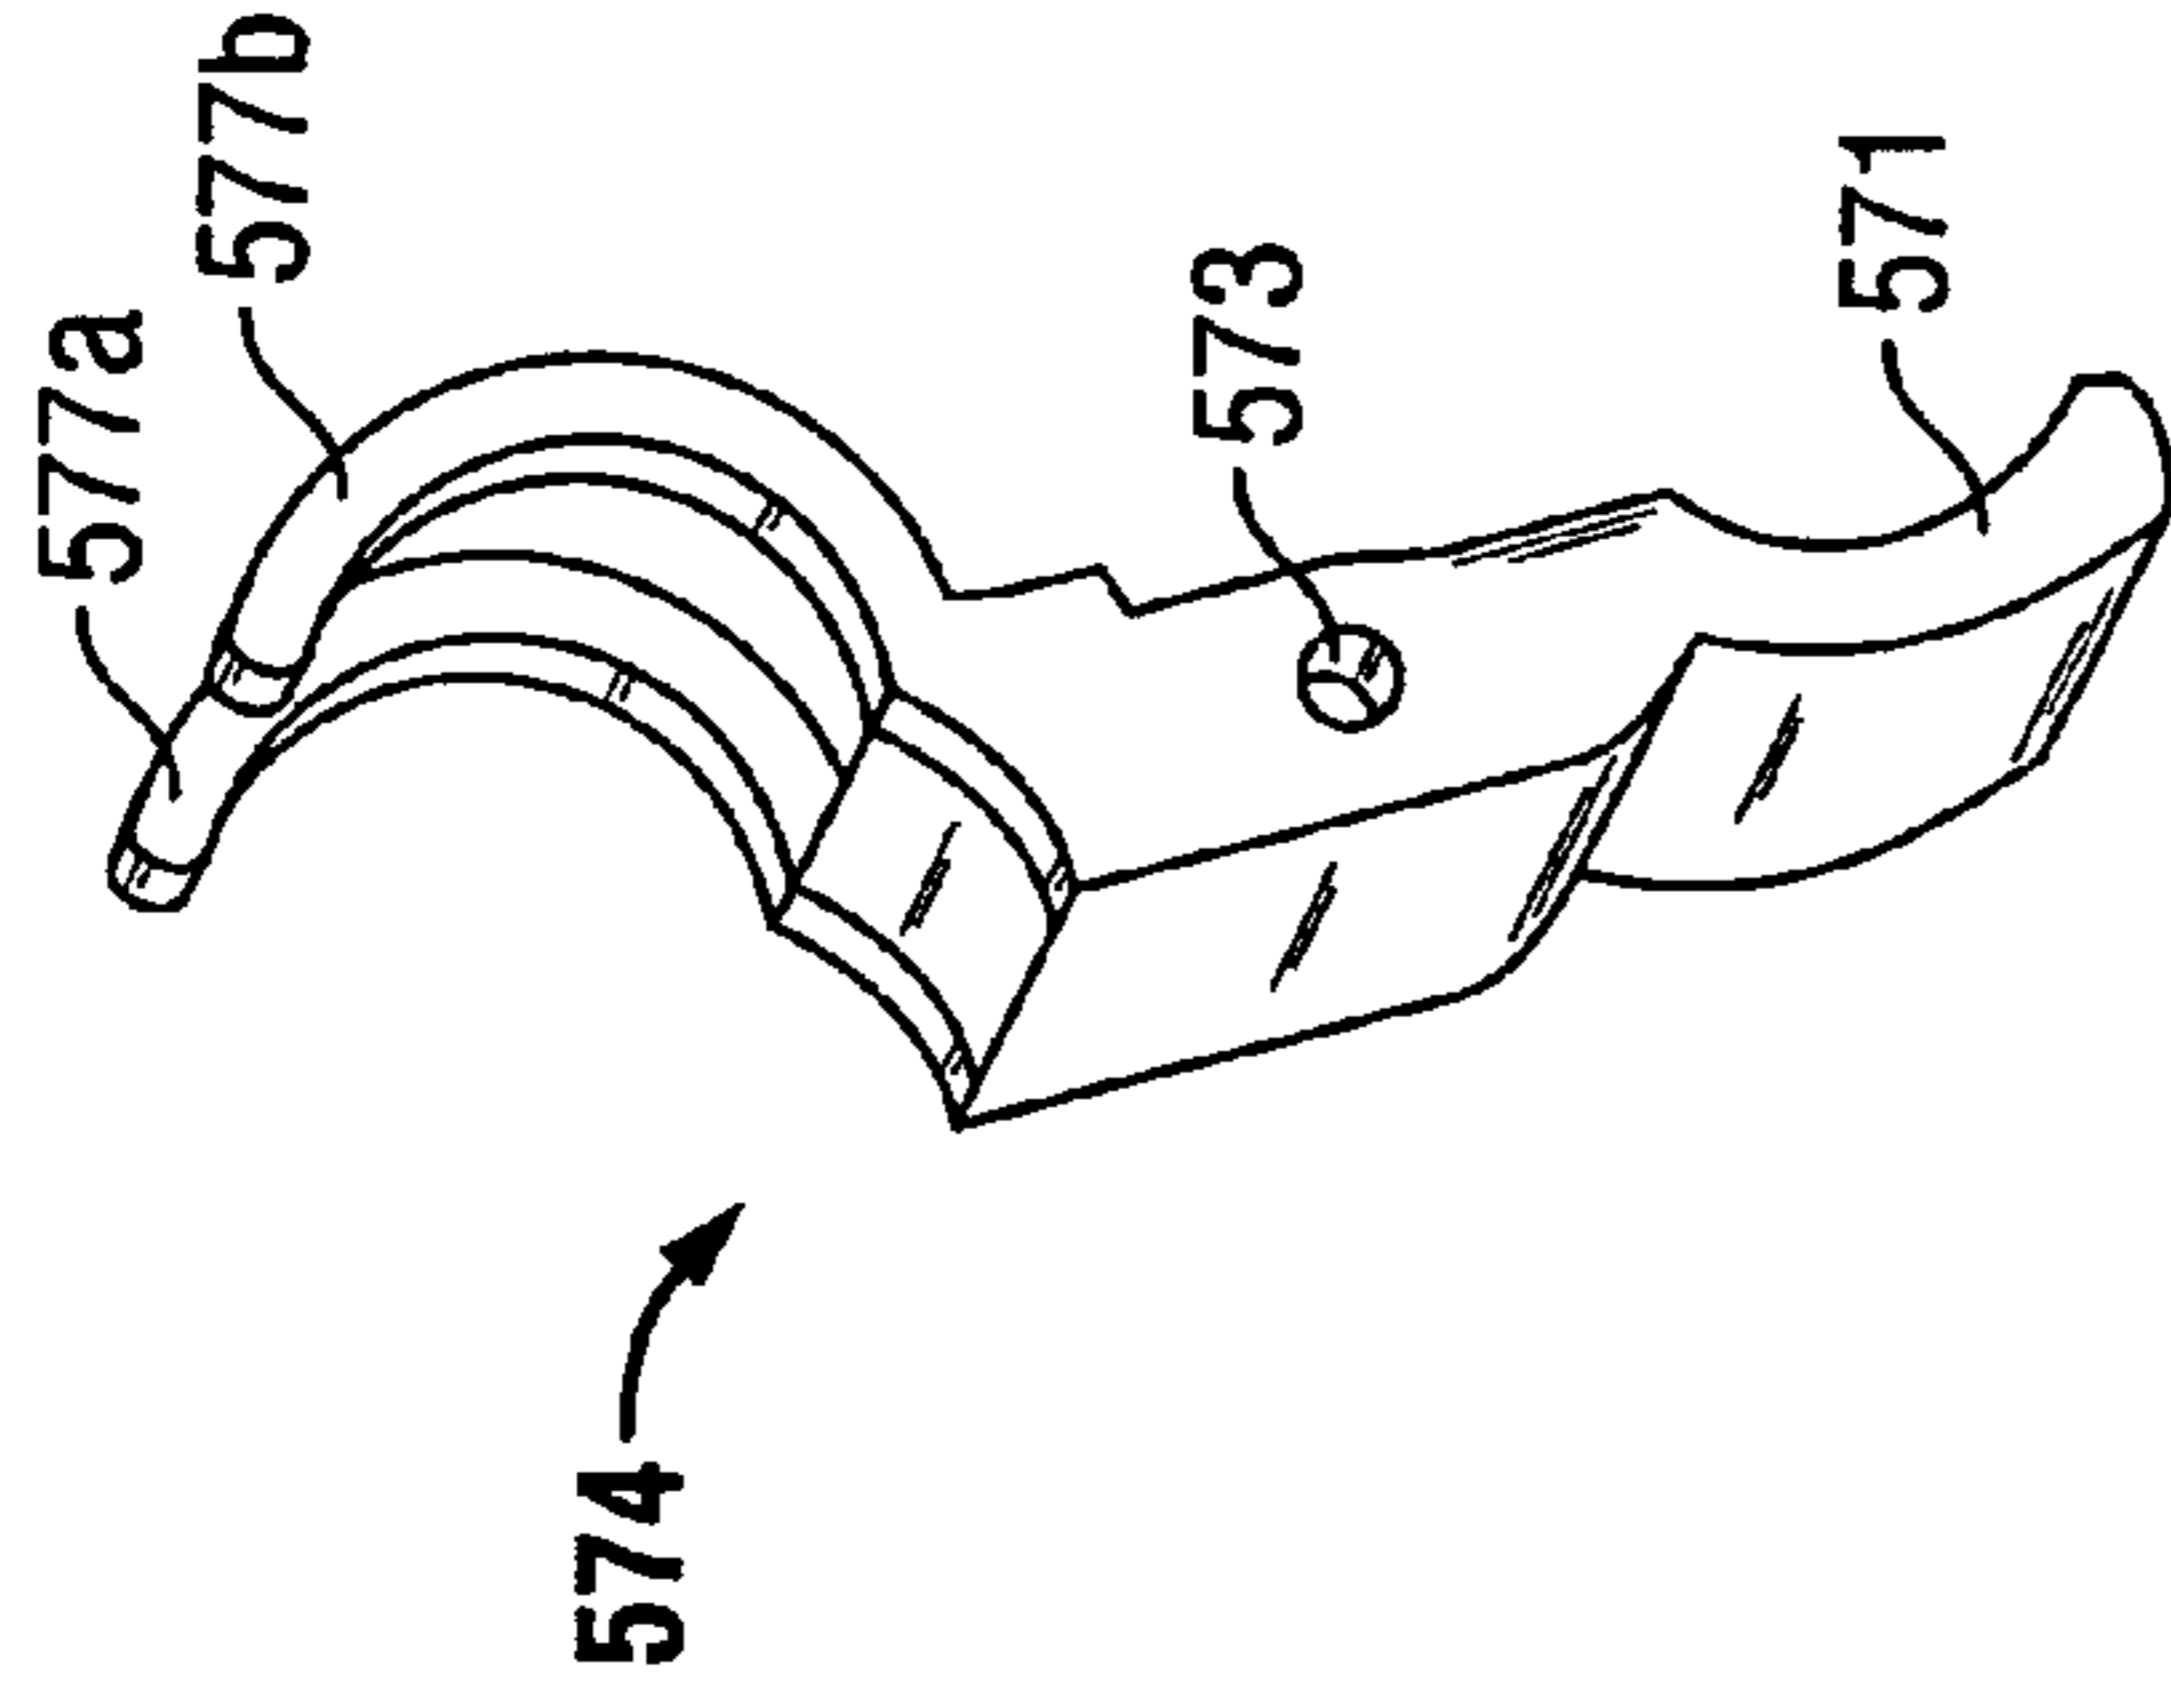


FIG. 50C

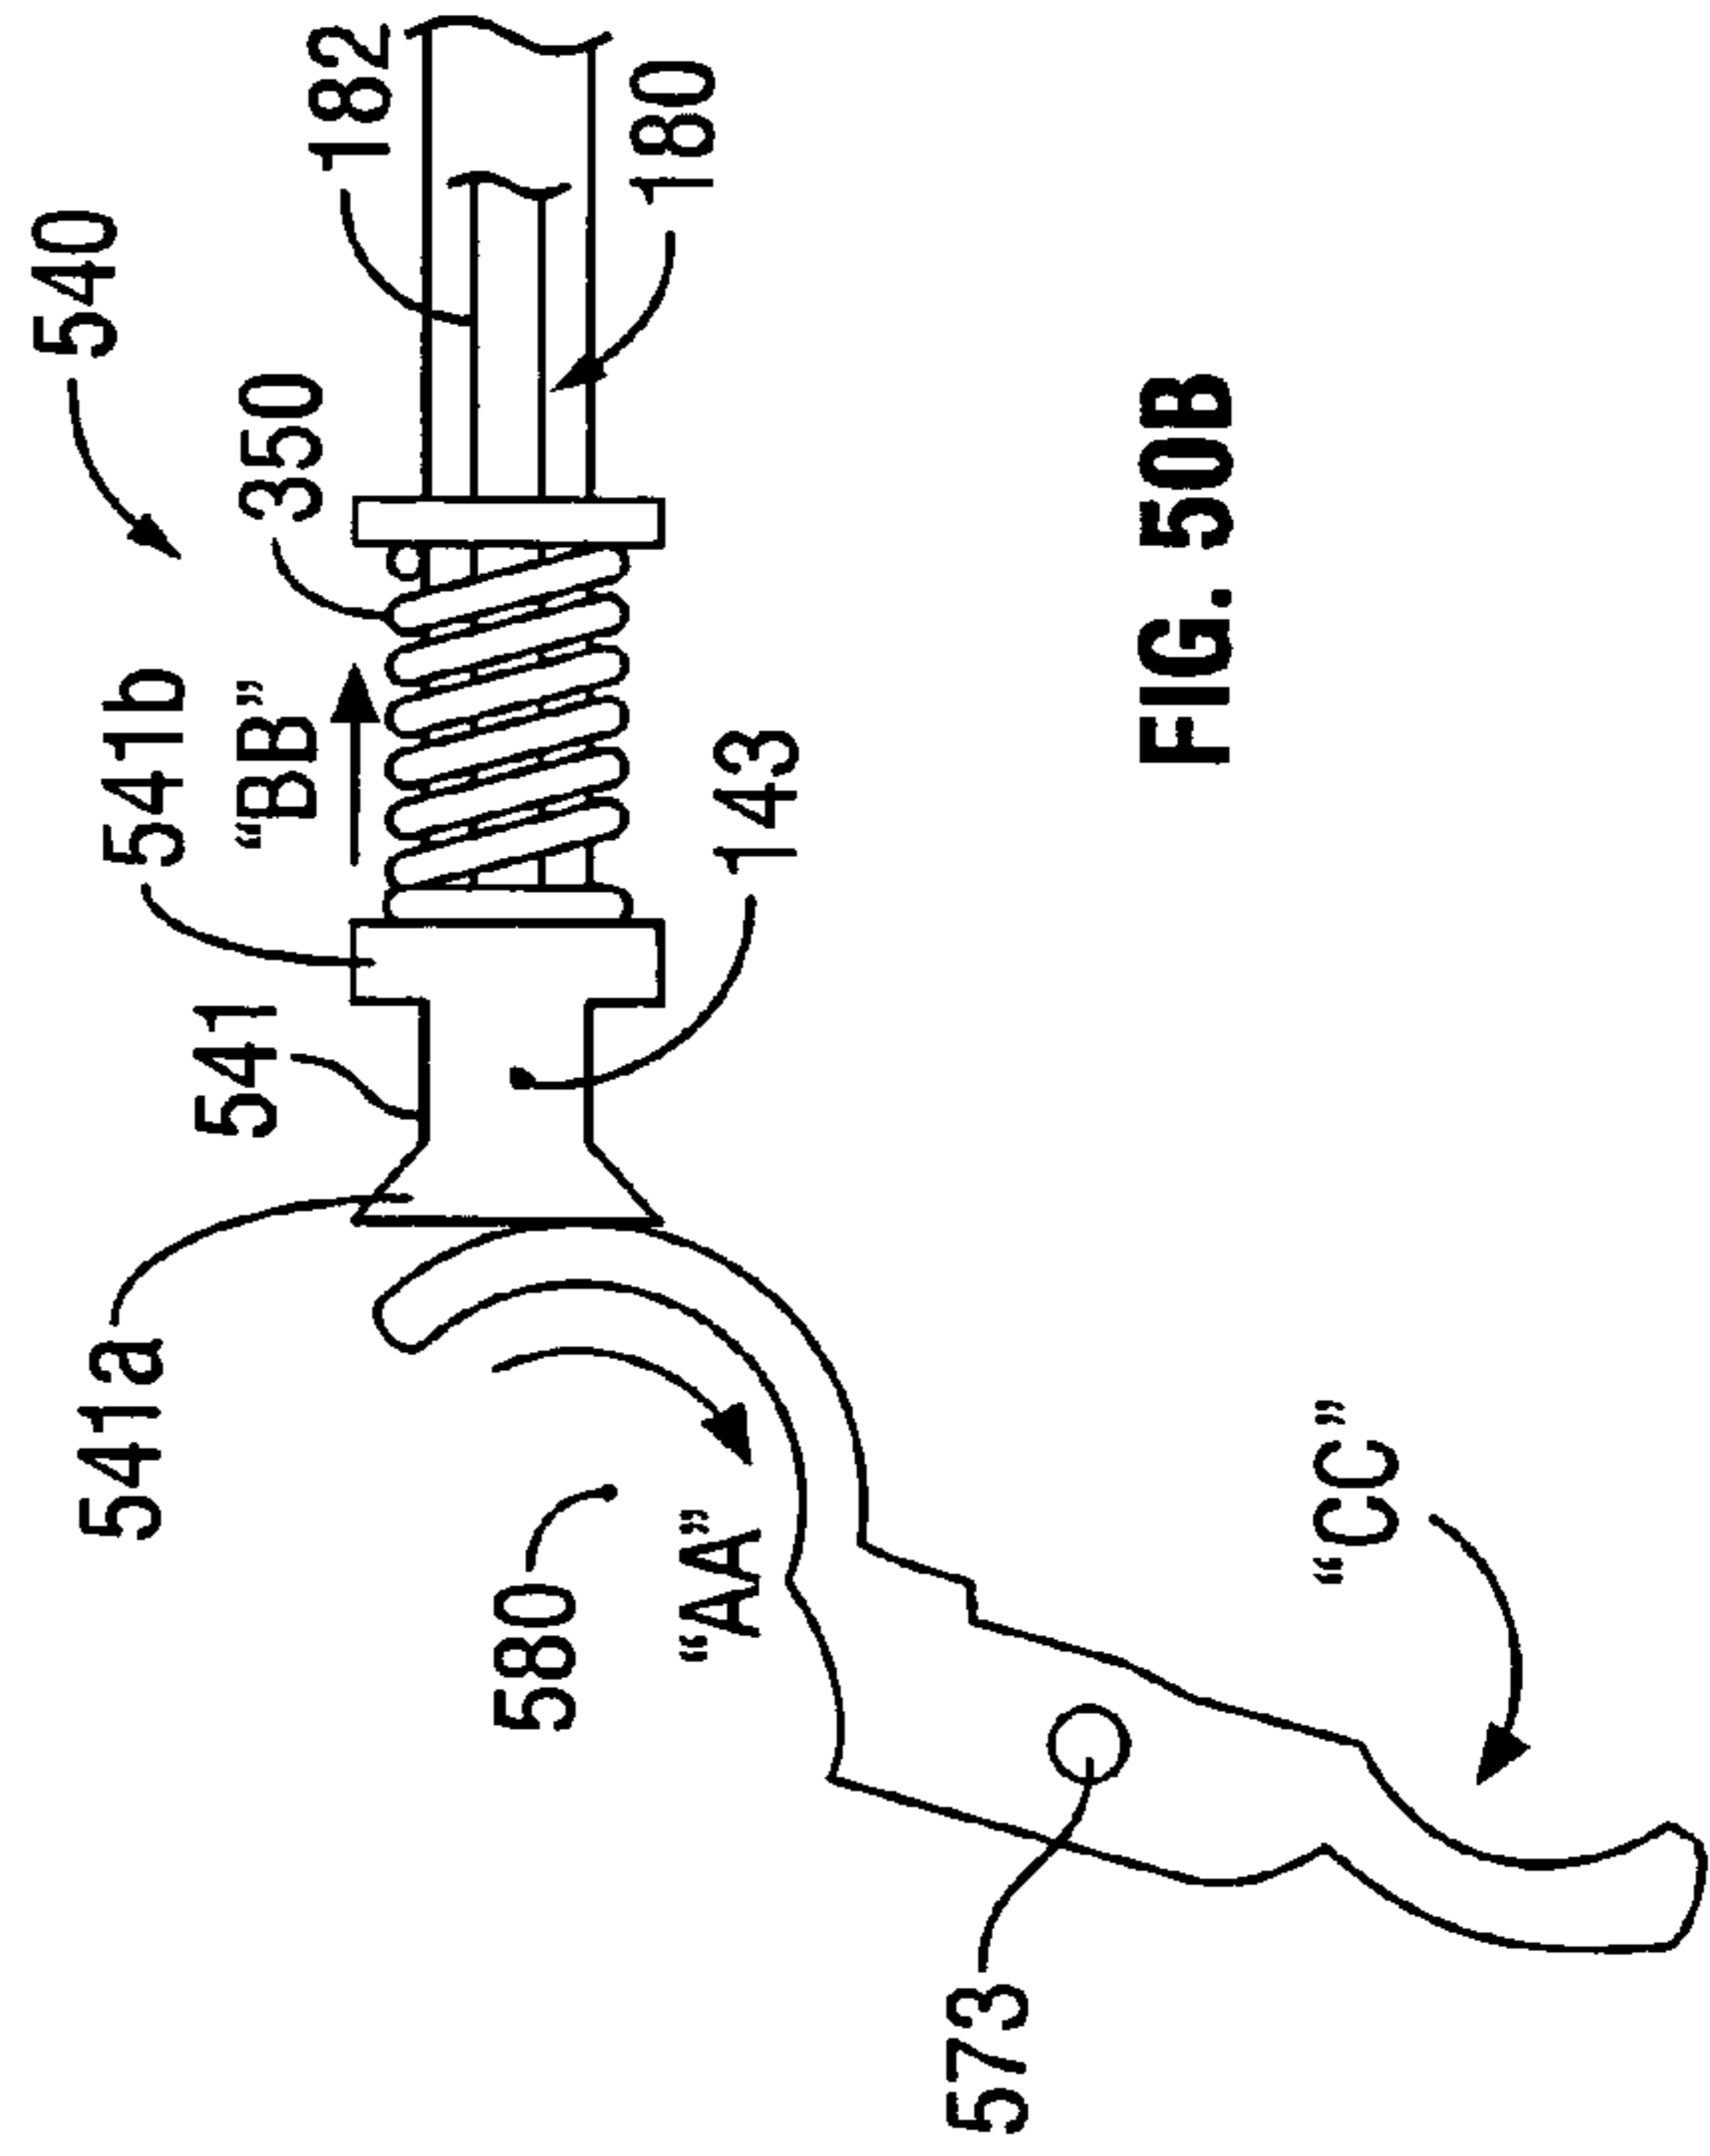


FIG. 50B

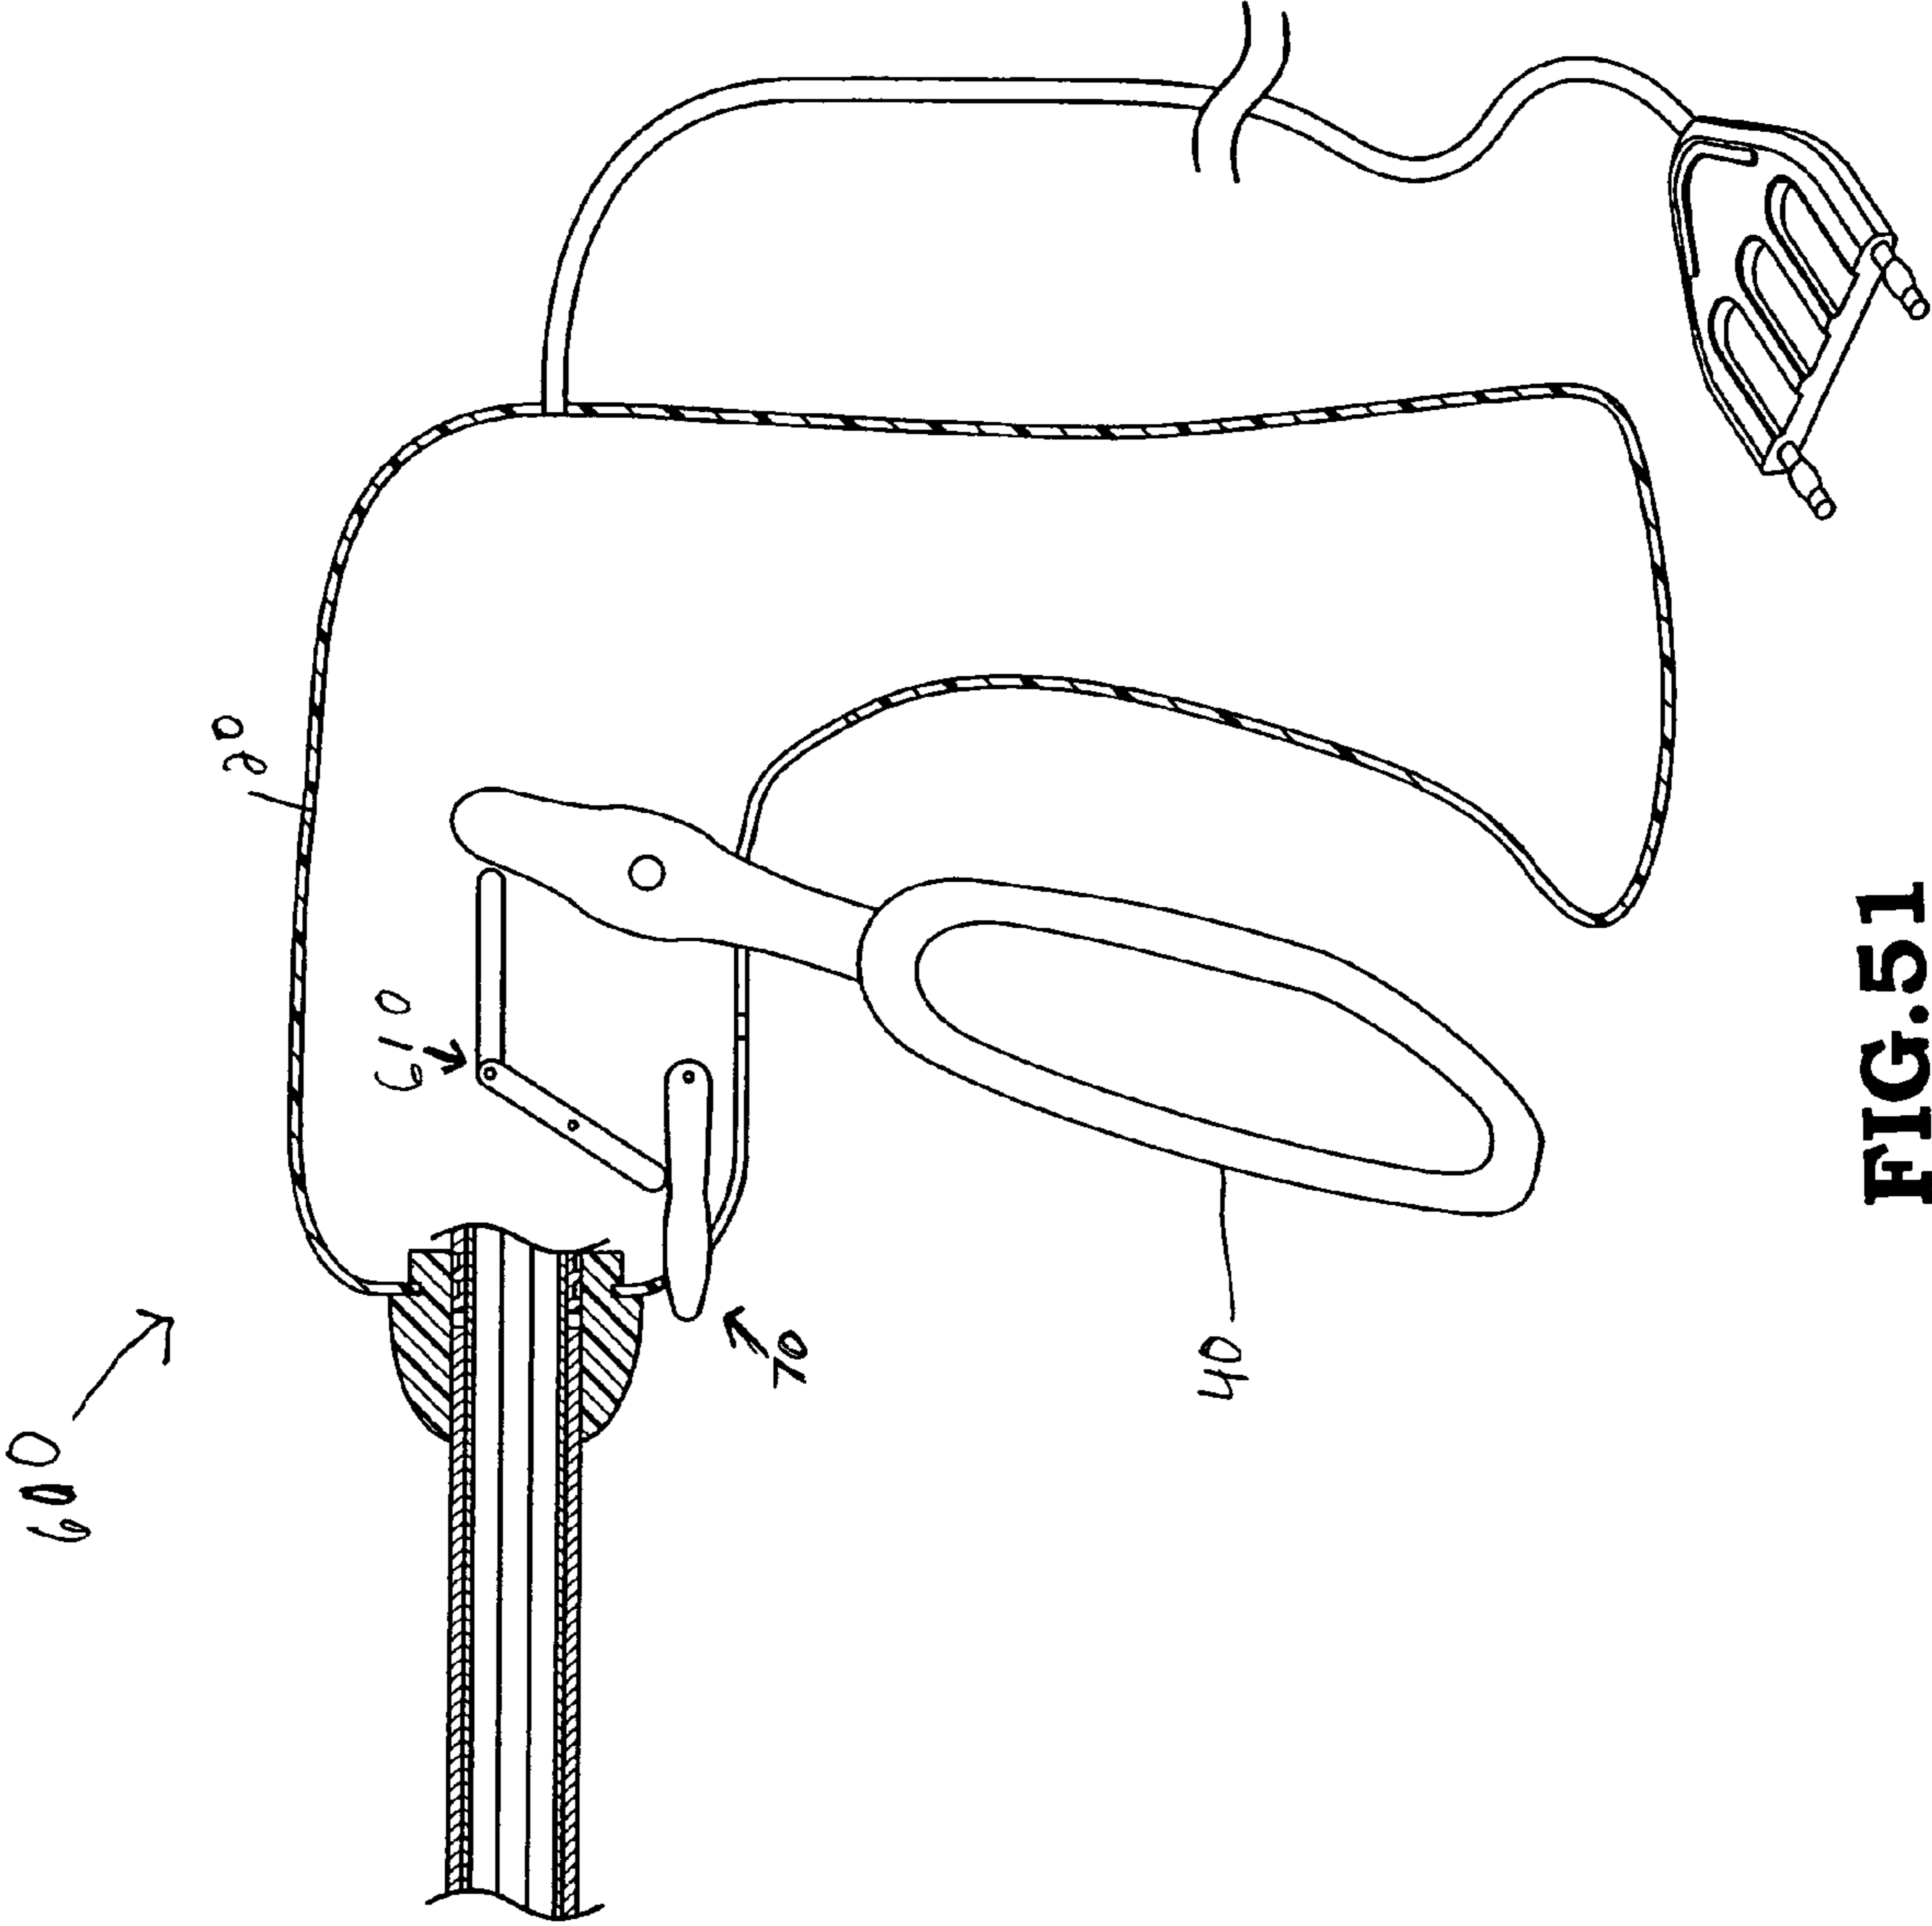


FIG. 51

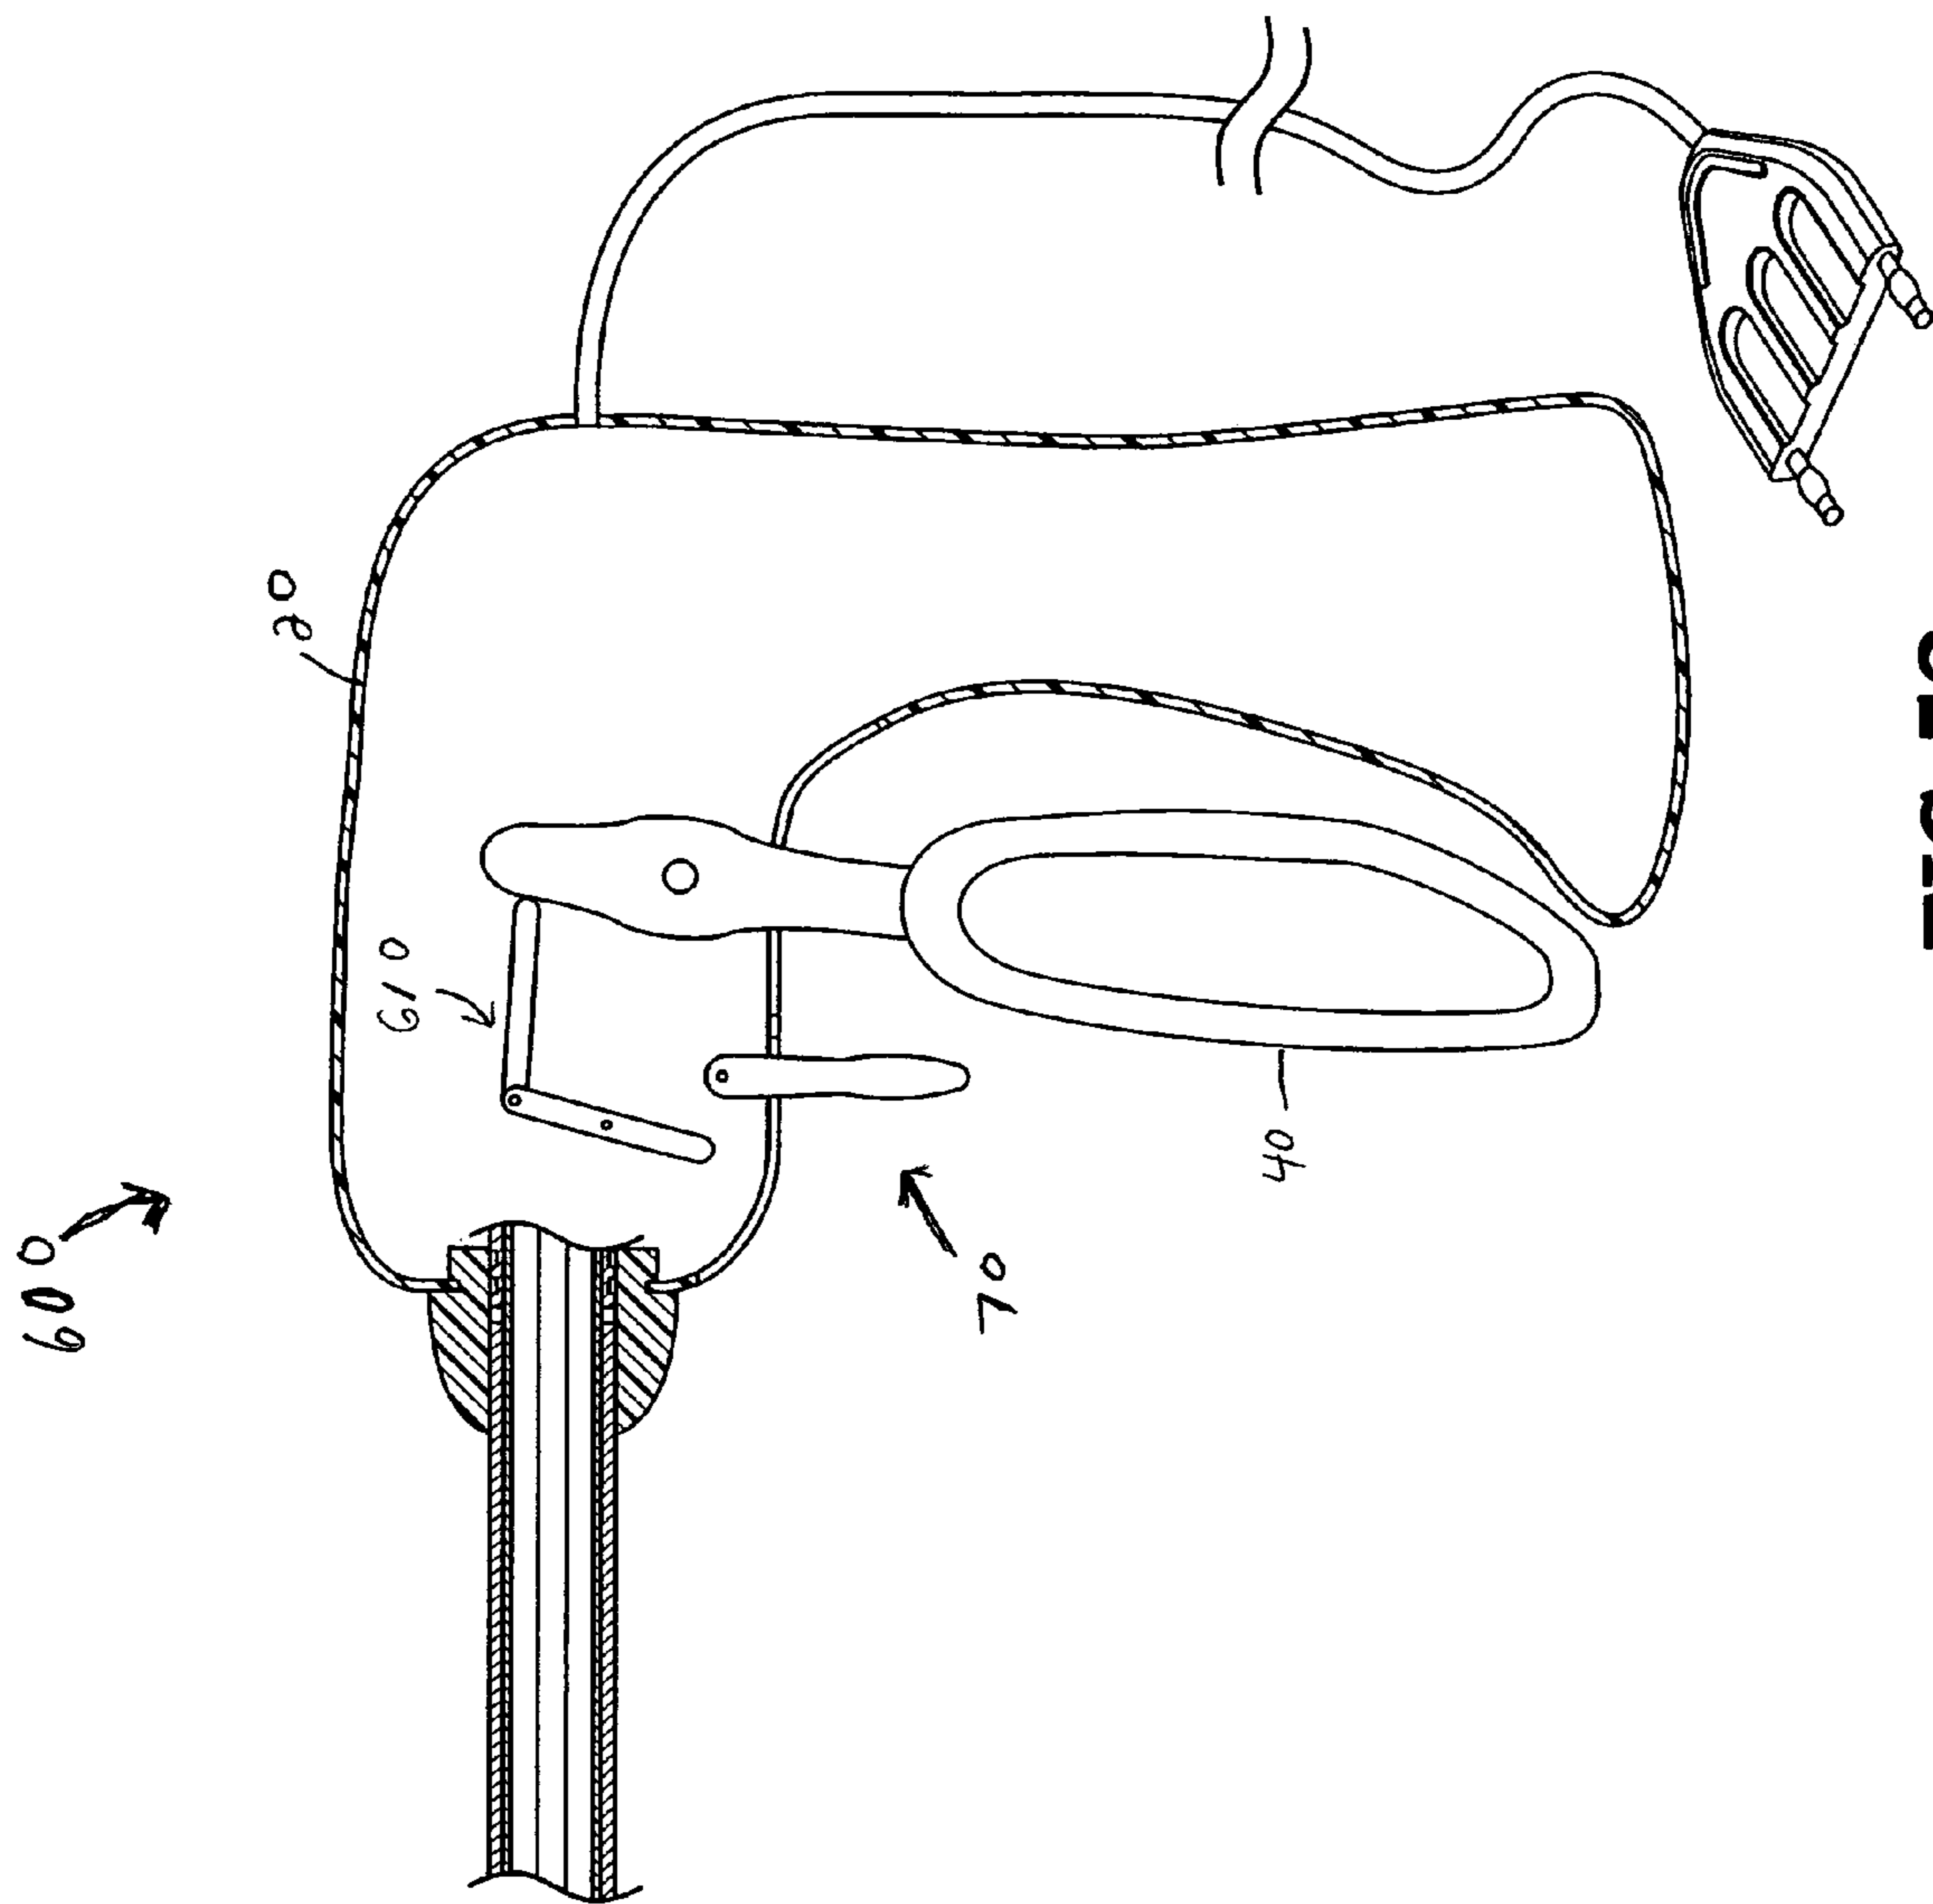


FIG. 52

1

**VESSEL SEALER AND DIVIDER HAVING
ELONGATED KNIFE STROKE AND SAFETY
CUTTING MECHANISM**

CROSS REFERENCE TO RELATED
APPLICATION

This application is a continuation-in-part of U.S. application Ser. No. 10/460,926 filed on Jun. 13, 2003 by Dycus, et al. entitled "VESSEL SEALER AND DIVIDER FOR USE WITH SMALL TROCARS AND CANNULAS", the entire contents of which are hereby incorporated by reference herein.

BACKGROUND

The present disclosure relates to an electrosurgical forceps and more particularly, the present disclosure relates to an endoscopic bipolar electrosurgical forceps for sealing and/or cutting tissue.

TECHNICAL FIELD

Electrosurgical forceps utilize both mechanical clamping action and electrical energy to effect hemostasis by heating the tissue and blood vessels to coagulate, cauterize and/or seal tissue. As an alternative to open forceps for use with open surgical procedures, many modern surgeons use endoscopes and endoscopic instruments for remotely accessing organs through smaller, puncture-like incisions. As a direct result thereof, patients tend to benefit from less scarring and reduced healing time.

Endoscopic instruments are inserted into the patient through a cannula, or port, which has been made with a trocar. Typical sizes for cannulas range from three millimeters to twelve millimeters. Smaller cannulas are usually preferred, which, as can be appreciated, ultimately presents a design challenge to instrument manufacturers who must find ways to make endoscopic instruments that fit through the smaller cannulas.

Many endoscopic surgical procedures require cutting or ligating blood vessels or vascular tissue. Due to the inherent spatial considerations of the surgical cavity, surgeons often have difficulty suturing vessels or performing other traditional methods of controlling bleeding, e.g., clamping and/or tying-off transected blood vessels. By utilizing an endoscopic electrosurgical forceps, a surgeon can either cauterize, coagulate/desiccate and/or simply reduce or slow bleeding simply by controlling the intensity, frequency and duration of the electrosurgical energy applied through the jaw members to the tissue. Most small blood vessels, i.e., in the range below two millimeters in diameter, can often be closed using standard electrosurgical instruments and techniques. However, if a larger vessel is ligated, it may be necessary for the surgeon to convert the endoscopic procedure into an open-surgical procedure and thereby abandon the benefits of endoscopic surgery. Alternatively, the surgeon can seal the larger vessel or tissue.

It is thought that the process of coagulating vessels is fundamentally different than electrosurgical vessel sealing. For the purposes herein, "coagulation" is defined as a process of desiccating tissue wherein the tissue cells are ruptured and dried. "Vessel sealing" or "tissue sealing" is defined as the process of liquefying the collagen in the tissue so that it reforms into a fused mass. Coagulation of small vessels is sufficient to permanently close them, while larger vessels need to be sealed to assure permanent closure.

2

In order to effectively seal larger vessels (or tissue) two predominant mechanical parameters must be accurately controlled—the pressure applied to the vessel (tissue) and the gap distance between the electrodes—both of which are affected by the thickness of the sealed vessel. More particularly, accurate application of pressure is important to oppose the walls of the vessel; to reduce the tissue impedance to a low enough value that allows enough electrosurgical energy through the tissue; to overcome the forces of expansion during tissue heating; and to contribute to the end tissue thickness which is an indication of a good seal. It has been determined that a typical fused vessel wall is optimum between 0.001 and 0.006 inches. Below this range, the seal may shred or tear and above this range the lumens may not be properly or effectively sealed.

With respect to smaller vessels, the pressure applied to the tissue tends to become less relevant whereas the gap distance between the electrically conductive surfaces becomes more significant for effective sealing. In other words, the chances of the two electrically conductive surfaces touching during activation increases as vessels become smaller.

Many known instruments include blade members or shearing members which simply cut tissue in a mechanical and/or electromechanical manner and are relatively ineffective for vessel sealing purposes. Other instruments rely on clamping pressure alone to procure proper sealing thickness and are not designed to take into account gap tolerances and/or parallelism and flatness requirements which are parameters which, if properly controlled, can assure a consistent and effective tissue seal. For example, it is known that it is difficult to adequately control thickness of the resulting sealed tissue by controlling clamping pressure alone for either of two reasons: 1) if too much force is applied, there is a possibility that the two poles will touch and energy will not be transferred through the tissue resulting in an ineffective seal; or 2) if too low a force is applied the tissue may pre-maturely move prior to activation and sealing and/or a thicker, less reliable seal may be created.

As mentioned above, in order to properly and effectively seal larger vessels or tissue, a greater closure force between opposing jaw members is required. It is known that a large closure force between the jaws typically requires a large moment about the pivot for each jaw. This presents a design challenge because the jaw members are typically affixed with pins which are positioned to have small moment arms with respect to the pivot of each jaw member. A large force, coupled with a small moment arm, is undesirable because the large forces may shear the pins. As a result, designers must compensate for these large closure forces by either designing instruments with metal pins and/or by designing instruments which at least partially offload these closure forces to reduce the chances of mechanical failure. As can be appreciated, if metal pivot pins are employed, the metal pins must be insulated to avoid the pin acting as an alternate current path between the jaw members which may prove detrimental to effective sealing.

Increasing the closure forces between electrodes may have other undesirable effects, e.g., it may cause the opposing electrodes to come into close contact with one another which may result in a short circuit and a small closure force may cause pre-mature movement of the tissue during compression and prior to activation. As a result thereof, providing an instrument which consistently provides the appropriate closure force between opposing electrode within a preferred pressure range will enhance the chances of a successful seal. As can be appreciated, relying on a surgeon to manually provide the appropriate closure force within the

appropriate range on a consistent basis would be difficult and the resultant effectiveness and quality of the seal may vary. Moreover, the overall success of creating an effective tissue seal is greatly reliant upon the user's expertise, vision, dexterity, and experience in judging the appropriate closure force to uniformly, consistently and effectively seal the vessel. In other words, the success of the seal would greatly depend upon the ultimate skill of the surgeon rather than the efficiency of the instrument.

It has been found that the pressure range for assuring a consistent and effective seal is between about 3 kg/cm² to about 16 kg/cm² and, preferably, within a working range of 7 kg/cm² to 13 kg/cm². Manufacturing an instrument which is capable of providing a closure pressure within this working range has been shown to be effective for sealing arteries, tissues and other vascular bundles.

Various force-actuating assemblies have been developed in the past for providing the appropriate closure forces to effect vessel sealing. For example, one such actuating assembly has been developed by Valleylab Inc., a division of Tyco Healthcare LP, for use with Valleylab's vessel sealing and dividing instrument commonly sold under the trademark LIGASURE ATLAS®. This assembly includes a four-bar mechanical linkage, a spring and a drive assembly which cooperate to consistently provide and maintain tissue pressures within the above working ranges. The LIGASURE ATLAS® is presently designed to fit through a 10 mm cannula and includes a bi-lateral jaw closure mechanism which is activated by a foot switch. A trigger assembly extends a knife distally to separate the tissue along the tissue seal. A rotating mechanism is associated with distal end of the handle to allow a surgeon to selectively rotate the jaw members to facilitate grasping tissue. Co-pending U.S. application Ser. Nos. 10/179,863 and 10/116,944 and PCT Application Serial Nos. PCT/US01/01890 and PCT/7201/11340 describe in detail the operating features of the LIGASURE ATLAS® and various methods relating thereto. The contents of all of these applications are hereby incorporated by reference herein.

It would be desirable to develop a smaller, simpler endoscopic vessel sealing instrument which can be utilized with a 5 mm cannula. Preferably, the instrument would include a simpler and more mechanically advantageous drive assembly to facilitate grasping and manipulating vessels and tissue. In addition, it would be desirable to manufacture an instrument which includes a hand switch and a unilateral jaw closure mechanism.

SUMMARY

The present disclosure relates to an endoscopic bipolar forceps which is designed to be utilized with a 5 mm trocar or cannula and includes a housing and a shaft affixed to the distal end of the housing. Preferably, the shaft includes a reduced diameter such that the shaft is freely insertable through the trocar. The shaft also includes a longitudinal axis defined therethrough and a pair of first and second jaw members attached to a distal end thereof. The forceps includes a drive assembly for moving the first jaw member relative to the second member from a first position wherein the jaw members are disposed in spaced relation relative to each other to a second position wherein the jaw members cooperate to grasp tissue therebetween. A movable handle is included which is rotatable about a pivot located above the longitudinal axis of the shaft. Movement of the handle engages a drive flange into mechanical cooperation with the drive assembly to move the jaw members from the open and

closed positions. Advantageously, the pivot is located a fixed distance above the longitudinal axis to provide lever-like mechanical advantage to the drive flange. The drive flange is located generally along the longitudinal axis. The forceps is connected to a source of electrosurgical energy which carries electrical potentials to each respective jaw member such that the jaw members are capable of conducting bipolar energy through tissue held therebetween to effect a tissue seal.

In yet another embodiment, the forceps includes a hand switch disposed within the housing which is electromechanically connected to the energy source. Advantageously, the hand switch allows a user to selectively supply bipolar energy to the jaw members to effect a tissue seal.

In one embodiment, the forceps includes a selectively advanceable knife assembly for cutting tissue in a forward direction along the tissue seal. A rotating assembly may also be included for rotating the jaw members about the longitudinal axis defined through the shaft. Advantageously, the rotating assembly is located proximal to the driving flange and near the hand switch to facilitate rotation.

Preferably, the movable jaw member includes a first electrical potential and the fixed jaw member includes a second electrical potential. A lead connects the movable jaw member to the first potential and a conductive tube (which is disposed through the shaft) conducts a second electrical potential to the fixed jaw member. Advantageously, the conductive tube is connected to the rotating assembly to permit selective rotation of the jaw members.

In one embodiment, the drive assembly includes a reciprocating sleeve which upon activation of the movable handle, translates atop the rotating conductive tube to move the movable jaw member relative to the fixed jaw member. Preferably, the movable jaw member includes a detent which extends beyond the fixed jaw member which is designed for engagement with the reciprocating sleeve such that, upon translation thereof, the movable jaw member moves relative to the fixed jaw member. Advantageously, a spring is included with the drive assembly to facilitate actuation of the movable handle and to assure the closure force is maintained within the working range of about 3 kg/cm² to about 16 kg/cm² and, preferably, about 7 kg/cm² to about 13 kg/cm².

Preferably, at least one of the jaw members includes a series of stop members disposed thereon for regulating the distance between the jaw members (i.e., creating a gap between the two opposing jaw members) during the sealing process. As can be appreciated, regulating the gap distance between opposing jaw members along with maintaining the closing pressure to within the above-described ranges will produce a reliable and consistent tissue seal.

The present disclosure also relates to an endoscopic bipolar forceps which includes a shaft having a movable jaw member and a fixed jaw member at a distal end thereof. The forceps also includes a drive assembly for moving the movable jaw member relative to the fixed jaw member from a first position wherein the movable jaw member is disposed in spaced relation relative to the fixed jaw member to a second position wherein the movable jaw member is closer to the fixed jaw member for manipulating tissue. A movable handle is included which actuates the drive assembly to move the movable jaw member.

The forceps connects to a source of electrosurgical energy which is conducted to each jaw member such that the jaw members are capable of conducting bipolar energy through tissue held therebetween to effect a tissue seal. Advantageously, the forceps also includes a selectively advanceable

knife assembly for cutting tissue in a distal direction along the tissue seal and a stop member disposed on at least one of the jaw members for regulating the distance between jaw members during sealing.

In another embodiment the present disclosure relates to an endoscopic bipolar forceps which includes a shaft having a movable jaw member and a fixed jaw member at a distal end thereof and a drive assembly for moving the movable jaw member relative to the fixed jaw member as described above. A movable handle is included for actuating the drive assembly to move the movable jaw member and the jaw members are each adapted to connect to a source of electrical energy such that the jaw members are capable of conducting energy through tissue held therebetween to effect a tissue seal. A trigger assembly is operatively disposed relative to the movable handle for selectively advancing a knife assembly for cutting tissue along the tissue seal. The knife assembly includes a generally donut-shaped knife collar which cooperates with a knife shaft to advance a knife through tissue upon activation of the trigger assembly.

Preferably, the trigger assembly includes a trigger and a flange having two C-shaped legs which are configured to abut a proximal end of the knife collar such that rotation of the trigger, in turn, rotates the C-shaped legs and urges the knife collar distally to advance the knife through tissue. A spring may be included for biasing the knife collar and the trigger assembly in a proximal, unactuated position. The radius of curvature of the C-shaped legs of the flange may be dimensioned according to the type of tissue being treated or depending upon a particular surgical purpose.

BRIEF DESCRIPTION OF THE DRAWINGS

Various embodiments of the subject instrument are described herein with reference to the drawings wherein:

FIG. 1 is a left, perspective view of an endoscopic bipolar forceps showing a housing, a shaft and an end effector assembly according to the present disclosure;

FIG. 2 is a top view of the forceps of FIG. 1;

FIG. 3 is a left, side view of the forceps of FIG. 1;

FIG. 4 is a left, perspective view of the forceps of FIG. 1 showing the rotation of the end effector assembly about a longitudinal axis "A";

FIG. 5 is a front view of the forceps of FIG. 1;

FIG. 6 is an enlarged view of the indicated area of detail of FIG. 5 showing an enhanced view of the end effector assembly detailing a pair of opposing jaw members;

FIG. 7 is an enlarged, rear perspective view of the housing;

FIG. 8 is an enlarged, left perspective view of the end effector assembly with the jaw members shown in open configuration;

FIG. 9 is an enlarged, side view of the end effector assembly;

FIG. 10 is an enlarged, perspective view of the underside of the upper jaw member of the end effector assembly;

FIG. 11 is an enlarged, broken perspective view showing the end effector assembly and highlighting a cam-like closing mechanism which cooperates with a reciprocating pull sleeve to move the jaw members relative to one another;

FIG. 12 is a full perspective view of the end effector assembly of FIG. 11;

FIG. 13 is an enlarged, perspective view of the housing and the internal working components thereof;

FIG. 14 is top, perspective view of the housing of FIG. 13 with parts separated;

FIG. 15 is a left, perspective view of a rotating assembly, drive assembly, knife assembly and lower jaw member according to the present disclosure;

FIG. 16 is a rear, perspective view of the rotating assembly, drive assembly and knife assembly;

FIG. 17 is an enlarged, top, perspective view of the end effector assembly with parts separated;

FIG. 18 is an enlarged, perspective view of the knife assembly;

FIG. 19 is an enlarged, perspective view of the rotating assembly;

FIG. 20 is an enlarged, perspective view of the drive assembly;

FIG. 21 is an enlarged, perspective view of the knife assembly with parts separated;

FIG. 22 is an enlarged view of the indicated area of detail of FIG. 21 showing a knife blade of the knife assembly;

FIG. 23 is a greatly-enlarged, perspective view of a distal end of the knife assembly;

FIG. 24 is a greatly-enlarged, perspective view of a knife drive of the knife assembly;

FIG. 25 is an enlarged, perspective view of the rotating assembly and lower jaw member with parts separated;

FIG. 26 is a cross section of the area indicated in detail in FIG. 25;

FIG. 27 is a greatly-enlarged, perspective view of the lower jaw member;

FIG. 28 is an enlarged, perspective view of the drive assembly;

FIG. 29 is an enlarged perspective view of the drive assembly of FIG. 28 with parts separated;

FIG. 30 is an internal, side view of the housing showing the inner-working components thereof;

FIG. 31 is a cross-section of the housing with the end effector shown in open configuration and showing the internal, electrical routing of an electrosurgical cable and electrical leads;

FIG. 32 is a greatly-enlarged view of the indicated area of detail of FIG. 31;

FIG. 33 is a greatly-enlarged view of the indicated area of detail of FIG. 31;

FIG. 34 is a greatly-enlarged, cross section of the shaft taken along line 34—34;

FIG. 35 is a side, cross section of the shaft and end effector assembly;

FIG. 36 is a perspective view showing the forceps of the present disclosure being utilized with a 5 mm cannula;

FIG. 37 is a side, cross section of the housing showing the moving components of the drive assembly during actuation;

FIG. 38 is a greatly-enlarged, perspective view of a handle locking mechanism for use with the drive assembly;

FIG. 39 is a greatly-enlarged view of the indicated area of detail in FIG. 37;

FIG. 40 is a greatly-enlarged view of the indicated area of detail in FIG. 37;

FIG. 41 is an enlarged, rear, perspective view of the end effectors shown grasping tissue;

FIG. 42 is an enlarged view of a tissue seal;

FIG. 43 is a side, cross section of a tissue seal;

FIG. 44 is a cross section of the housing with the handle in a locked configuration and showing the moving components of the knife assembly during activation;

FIG. 45 is an enlarged view of the area indicated in detail in FIG. 44;

FIG. 46 is a side, cross section of a tissue seal after separation by the knife assembly;

FIG. 47 is a side, cross section of the housing showing the release of the knife assembly and release of the drive assembly to open the jaw members and release the tissue;

FIG. 48 is a greatly-enlarged view of the indicated area of detail in FIG. 47;

FIG. 49 is a greatly-enlarged view of the indicated area of detail in FIG. 47;

FIG. 50A is an enlarged side view of alternate embodiments of the knife assembly and trigger assembly which are designed to improve the overall stroke length of the knife blade for cutting tissue;

FIG. 50B is an enlarged side view of the knife assembly and trigger assembly of FIG. 50A shown in an actuated position;

FIG. 50C is an enlarged perspective view of the trigger assembly of FIG. 50A;

FIG. 51 is a schematic, cross-sectional view of a forceps similar to the forceps of FIG. 1 showing a safety mechanism with the trigger assembly in a locked configuration; and

FIG. 52 is the forceps of FIG. 51, showing the safety mechanism with the trigger assembly in an unlocked configuration.

DETAILED DESCRIPTION

Turning now to FIGS. 1–3, one embodiment of an endoscopic bipolar forceps 10 is shown for use with various surgical procedures and generally includes a housing 20, a handle assembly 30, a rotating assembly 80, a trigger assembly 70 and an end effector assembly 100 which mutually cooperate to grasp, seal and divide tubular vessels and vascular tissue 420 (FIG. 36). Although the majority of the figure drawings depict a bipolar forceps 10 for use in connection with endoscopic surgical procedures, the present disclosure may be used for more traditional open surgical procedures. For the purposes herein, the forceps 10 is described in terms of an endoscopic instrument, however, it is contemplated that an open version of the forceps may also include the same or similar operating components and features as described below.

Forceps 10 includes a shaft 12 which has a distal end 16 dimensioned to mechanically engage the end effector assembly 100 and a proximal end 14 which mechanically engages the housing 20. Details of how the shaft 12 connects to the end effector are described in more detail below with respect to FIG. 25. The proximal end 14 of shaft 12 is received within the housing 20 and the connections relating thereto are described in detail below with respect to FIGS. 13 and 14. In the drawings and in the descriptions which follow, the term “proximal”, as is traditional, will refer to the end of the forceps 10 which is closer to the user, while the term “distal” will refer to the end which is further from the user.

As best seen in FIG. 1, forceps 10 also includes an electro-surgical cable 310 which connects the forceps 10 to a source of electro-surgical energy, e.g., a generator (not shown). Preferably, generators such as those sold by Valleylab—a division of Tyco Healthcare LP, located in Boulder Colo. are used as a source of electro-surgical energy, e.g., FORCE EZ™ Electro-surgical Generator, FORCE FX™ Electro-surgical Generator, FORCE 1C™, FORCE 2™ Generator, SurgiStat™ II. One such system is described in commonly-owned U.S. Pat. No. 6,033,399 entitled “ELECTROSURGICAL GENERATOR WITH ADAPTIVE POWER CONTROL” the entire contents of which are hereby incorporated by reference herein. Other systems have been described in commonly-owned U.S. Pat. No. 6,187,003 entitled “BIPOLAR ELECTROSURGICAL INSTRU-

MENT FOR SEALING VESSELS” the entire contents of which is also incorporated by reference herein.

Preferably, the generator includes various safety and performance features including isolated output, independent activation of accessories. Preferably, the electro-surgical generator includes Valleylab’s Instant Response™ technology features which provides an advanced feedback system to sense changes in tissue 200 times per second and adjust voltage and current to maintain appropriate power. The Instant Response™ technology is believed to provide one or more of the following benefits to surgical procedure: Consistent clinical effect through all tissue types; Reduced thermal spread and risk of collateral tissue damage; Less need to “turn up the generator”; and Designed for the minimally invasive environment.

Cable 310 is internally divided into cable lead 310a, 310b and 310c which each transmit electro-surgical energy through their respective feed paths through the forceps 10 to the end effector assembly 100 as explained in more detail below with respect to FIGS. 14 and 30.

Handle assembly 30 includes a fixed handle 50 and a movable handle 40. Fixed handle 50 is integrally associated with housing 20 and handle 40 is movable relative to fixed handle 50 as explained in more detail below with respect to the operation of the forceps 10. Rotating assembly 80 is preferably integrally associated with the housing 20 and is rotatable approximately 180 degrees in either direction about a longitudinal axis “A” (See FIG. 4). Details of the rotating assembly 80 are described in more detail with respect to FIGS. 13, 14, 15 and 16.

As best seen in FIGS. 2, 13 and 14, housing 20 is formed from two (2) housing halves 20a and 20b which each include a plurality of interfaces 27a–27f which are dimensioned to mechanically align and engage one another to form housing 20 and enclose the internal working components of forceps 10. As can be appreciated, fixed handle 50 which, as mentioned above, is integrally associated with housing 20, takes shape upon the assembly of the housing halves 20a and 20b.

It is envisioned that a plurality of additional interfaces (not shown) may be disposed at various points around the periphery of housing halves 20a and 20b for ultrasonic welding purposes, e.g., energy direction/deflection points. It is also contemplated that housing halves 20a and 20b (as well as the other components described below) may be assembled together in any fashion known in the art. For example, alignment pins, snap-like interfaces, tongue and groove interfaces, locking tabs, adhesive ports, etc. may all be utilized either alone or in combination for assembly purposes.

Rotating assembly 80 includes two halves 82a and 82b which, when assembled, form the rotating assembly 80 which, in turn, houses the drive assembly 150 and the knife assembly 140 (See FIGS. 13, 14 and 25). Half 80a includes a series of detents/flanges 375a, 375b, 375c and 375d (FIG. 25) which are dimensioned to engage a pair of corresponding sockets or other mechanical interfaces (not shown) disposed within rotating half 80a. Movable handle 40 and trigger assembly 70 are preferably of unitary construction and are operatively connected to the housing 20 and the fixed handle 50 during the assembly process.

As mentioned above, end effector assembly 100 is attached at the distal end 14 of shaft 12 and includes a pair of opposing jaw members 110 and 120. Movable handle 40 of handle assembly 30 is ultimately connected to a drive assembly 150 which, together, mechanically cooperate to impart movement of the jaw members 110 and 120 from an

open position wherein the jaw members **110** and **120** are disposed in spaced relation relative to one another, to a clamping or closed position wherein the jaw members **110** and **120** cooperate to grasp tissue **420** (FIG. **36**) therebetween.

It is envisioned that the forceps **10** may be designed such that it is fully or partially disposable depending upon a particular purpose or to achieve a particular result. For example, end effector assembly **100** may be selectively and releasably engageable with the distal end **16** of the shaft **12** and/or the proximal end **14** of shaft **12** may be selectively and releasably engageable with the housing **20** and the handle assembly **30**. In either of these two instances, the forceps **10** would be considered “partially disposable” or “reposable”, i.e., a new or different end effector assembly **100** (or end effector assembly **100** and shaft **12**) selectively replaces the old end effector assembly **100** as needed. As can be appreciated, the presently disclosed electrical connections would have to be altered to modify the instrument to a reposable forceps.

Turning now to the more detailed features of the present disclosure as described with respect to FIGS. **1–14**, movable handle **40** includes a finger loop **41** which has an aperture **42** defined therethrough which enables a user to grasp and move the handle **40** relative to the fixed handle **50**. Handle **40** also includes an ergonomically-enhanced gripping element **43** disposed along the inner peripheral edge of aperture **42** which is designed to facilitate gripping of the movable handle **40** during activation. It is envisioned that gripping element **43** may include one or more protuberances, scallops and/or ribs to enhance gripping. As best seen in FIG. **14**, movable handle **40** is selectively moveable about a pair of pivot pins **29a** and **29b** from a first position relative to fixed handle **50** to a second position in closer proximity to the fixed handle **50** which, as explained below, imparts movement of the jaw members **110** and **120** relative to one another. The movable handle include a clevis **45** which forms a pair of upper flanges **45a** and **45b** each having an aperture **49a** and **49b**, respectively, at an upper end thereof for receiving the pivot pins **29a** and **29b** therethrough and mounting the upper end of the handle **40** to the housing **20**. In turn, each pin **29a** and **29b** mounts to a respective housing half **20a** and **20b**.

Each upper flange **45a** and **45b** also includes a force-actuating flange or drive flange **47a** and **47b**, respectively, which are aligned along longitudinal axis “A” and which abut the drive assembly **150** such that pivotal movement of the handle **40** forces actuating flange against the drive assembly **150** which, in turn, closes the jaw members **110** and **120**. For the purposes herein, **47a** and **47b** which act simultaneously on the drive assembly are referred to as “driving flange **47**”. A more detailed explanation of the inter-cooperating components of the handle assembly **30** and the drive assembly **150** is discussed below.

As best seen in FIG. **14**, the lower end of the movable handle **40** includes a flange **90** which is preferably mounted to the movable handle **40** by pins **94a** and **94b** which engage a corresponding pair of apertures **91a** and **91b** disposed within the lower portion of handle **40** and apertures **97a** and **97b** disposed within flange **90**, respectively. Other methods of engagement are also contemplated, snap-lock, spring tab, etc. Flange **90** also includes a t-shaped distal end **95** which rides within a predefined channel **51** disposed within fixed handle **50** to lock the movable handle **40** relative to the fixed handle **50**. Additional features with respect to the t-shaped end **95** are explained below in the detailed discussion of the operational features of the forceps **10**.

Movable handle **40** is designed to provide a distinct mechanical advantage over conventional handle assemblies due to the unique position of the pivot pins **29a** and **29b** (i.e., pivot point) relative to the longitudinal axis “A” of the shaft **12** and the disposition of the driving flange **47** along longitudinal axis “A”. In other words, it is envisioned that by positioning the pivot pins **29a** and **29b** above the driving flange **47**, the user gains lever-like mechanical advantage to actuate the jaw members **110** and **120** enabling the user to close the jaw members **110** and **120** with lesser force while still generating the required forces necessary to effect a proper and effective tissue seal. It is also envisioned that the unilateral design of the end effector assembly **100** will also increase mechanical advantage as explained in more detail below.

As shown best in FIGS. **6–12**, the end effector assembly **100** includes opposing jaw members **110** and **120** which cooperate to effectively grasp tissue **420** for sealing purposes. The end effector assembly **100** is designed as a unilateral assembly, i.e., jaw member **120** is fixed relative to the shaft **12** and jaw member **110** pivots about a pivot pin **103** to grasp tissue **420**.

More particularly, the unilateral end effector assembly **100** includes one stationary or fixed jaw member **120** mounted in fixed relation to the shaft **12** and pivoting jaw member **110** mounted about a pivot pin **103** attached to the stationary jaw member **120**. A reciprocating sleeve **60** is slidingly disposed within the shaft **12** and is remotely operable by the drive assembly **150**. The pivoting jaw member **110** includes a detent or protrusion **117** which extends from jaw member **110** through an aperture **62** disposed within the reciprocating sleeve **60** (FIG. **12**). The pivoting jaw member **110** is actuated by sliding the sleeve **60** axially within the shaft **12** such that a distal end **63** of the aperture **62** abuts against the detent **117** on the pivoting jaw member **110** (See FIGS. **11** and **12**). Pulling the sleeve **60** proximally closes the jaw members **110** and **120** about tissue **420** grasped therebetween and pushing the sleeve **60** distally opens the jaw members **110** and **120** for grasping purposes.

As best illustrated in FIGS. **8** and **10**, a knife channel **115a** and **115b** runs through the center of the jaw members **110** and **120**, respectively, such that a blade **185** from the knife assembly **140** can cut the tissue **420** grasped between the jaw members **110** and **120** when the jaw members **110** and **120** are in a closed position. More particularly, the blade **185** can only be advanced through the tissue **420** when the jaw members **110** and **120** are closed thus preventing accidental or premature activation of the blade **185** through the tissue **420**. Put simply, the knife channel **115** (made up of half channels **115a** and **115b**) is blocked when the jaws members **110** and **120** are opened and aligned for distal activation when the jaw members **110** and **120** are closed (See FIGS. **35** and **39**). It is also envisioned that the unilateral end effector assembly **100** may be structured such that electrical energy can be routed through the sleeve **60** at the protrusion **117** contact point with the sleeve **60** or using a “brush” or lever (not shown) to contact the back of the moving jaw member **110** when the jaw member **110** closes. In this instance, the electrical energy would be routed through the protrusion **117** to the stationary jaw member **120**. Alternatively, the cable lead **311** may be routed to energize the stationary jaw member **120** and the other electrical potential may be conducted through the sleeve **60** and transferred to the pivoting jaw member **110** which establishes electrical continuity upon retraction of the sleeve **60**. It is envisioned that this particular envisioned embodiment will provide at least two important safety features: 1) the blade **185** cannot

extend while the jaw members **110** and **120** are opened; and 2) electrical continuity to the jaw members **110** and **120** is made only when the jaw members are closed. The illustrated forceps **10** only includes the novel knife channel **115**.

As best shown in FIG. **8**, jaw member **110** also includes a jaw housing **116** which has an insulative substrate or insulator **114** and an electrically conductive surface **112**. Insulator **114** is preferably dimensioned to securely engage the electrically conductive sealing surface **112**. This may be accomplished by stamping, by overmolding, by overmolding a stamped electrically conductive sealing plate and/or by overmolding a metal injection molded seal plate. For example and as shown in FIG. **17**, the electrically conductive sealing plate **112** includes a series of upwardly extending flanges **111a** and **111b** which are designed to matingly engage the insulator **114**. The insulator **114** includes a shoe-like interface **107** disposed at a distal end thereof which is dimensioned to engage the outer periphery **116a** of the housing **116** in a slip-fit manner. The shoe-like interface **107** may also be overmolded about the outer periphery of the jaw **110** during a manufacturing step. It is envisioned that lead **311** terminates within the shoe-like interface **107** at the point where lead **311** electrically connects to the seal plate **112** (not shown). The movable jaw member **110** also includes a wire channel **113** which is designed to guide cable lead **311** into electrical continuity with sealing plate **112** as described in more detail below.

All of these manufacturing techniques produce jaw member **110** having an electrically conductive surface **112** which is substantially surrounded by an insulating substrate **114**. The insulator **114**, electrically conductive sealing surface **112** and the outer, non-conductive jaw housing **116** are preferably dimensioned to limit and/or reduce many of the known undesirable effects related to tissue sealing, e.g., flashover, thermal spread and stray current dissipation. Alternatively, it is also envisioned that the jaw members **110** and **120** may be manufactured from a ceramic-like material and the electrically conductive surface(s) **112** are coated onto the ceramic-like jaw members **110** and **120**.

Jaw member **110** includes a pivot flange **118** which includes protrusion **117**. Protrusion **117** extends from pivot flange **118** and includes an arcuately-shaped inner surface **111** dimensioned to matingly engage the aperture **62** of sleeve **60** upon retraction thereof. Pivot flange **118** also includes a pin slot **119** which is dimensioned to engage pivot pin **103** to allow jaw member **110** to rotate relative to jaw member **120** upon retraction of the reciprocating sleeve **60**. As explained in more detail below, pivot pin **103** also mounts to the stationary jaw member **120** through a pair of apertures **101a** and **101b** disposed within a proximal portion of the jaw member **120**.

It is envisioned that the electrically conductive sealing surface **112** may also include an outer peripheral edge which has a pre-defined radius and the insulator **114** meets the electrically conductive sealing surface **112** along an adjoining edge of the sealing surface **112** in a generally tangential position. Preferably, at the interface, the electrically conductive surface **112** is raised relative to the insulator **114**. These and other envisioned embodiments are discussed in co-pending, commonly assigned Application Serial No. PCT/US01/11412 entitled "ELECTROSURGICAL INSTRUMENT WHICH REDUCES COLLATERAL DAMAGE TO ADJACENT TISSUE" by Johnson et al. and co-pending, commonly assigned Application Serial No. PCT/US01/11411 entitled "ELECTROSURGICAL INSTRUMENT WHICH IS DESIGNED TO REDUCE THE INCIDENCE OF FLASHOVER" by Johnson et al.

Preferably, the electrically conductive surface **112** and the insulator **114**, when assembled, form a longitudinally-oriented slot **115a** defined therethrough for reciprocation of the knife blade **185**. It is envisioned that the knife channel **115a** cooperates with a corresponding knife channel **115b** defined in stationary jaw member **120** to facilitate longitudinal extension of the knife blade **185** along a preferred cutting plane to effectively and accurately separate the tissue **420** along the formed tissue seal **450** (See FIGS. **42** and **46**).

Jaw member **120** includes similar elements to jaw member **110** such as jaw housing **126** having an insulator **124** and an electrically conductive sealing surface **122** which is dimensioned to securely engage the insulator **124**. Likewise, the electrically conductive surface **122** and the insulator **124**, when assembled, include a longitudinally-oriented channel **115a** defined therethrough for reciprocation of the knife blade **185**. As mentioned above, when the jaw members **110** and **120** are closed about tissue **420**, knife channels **115a** and **115b** form a complete knife channel **115** to allow longitudinal extension of the knife **185** in a distal fashion to sever tissue **420** along the tissue seal **450**. It is also envisioned that the knife channel **115** may be completely disposed in one of the two jaw members, e.g., jaw member **120**, depending upon a particular purpose. It is envisioned that the fixed jaw member **120** may be assembled in a similar manner as described above with respect to jaw member **110**.

As best seen in FIG. **8**, jaw member **120** includes a series of stop members **750** preferably disposed on the inner facing surfaces of the electrically conductive sealing surface **122** to facilitate gripping and manipulation of tissue and to define a gap "G" (FIG. **24**) between opposing jaw members **110** and **120** during sealing and cutting of tissue. It is envisioned that the series of stop members **750** may be employed on one or both jaw members **110** and **120** depending upon a particular purpose or to achieve a desired result. A detailed discussion of these and other envisioned stop members **750** as well as various manufacturing and assembling processes for attaching and/or affixing the stop members **750** to the electrically conductive sealing surfaces **112**, **122** are described in commonly-assigned, co-pending U.S. Application Serial No. PCT/US01/11413 entitled "VESSEL SEALER AND DIVIDER WITH NON-CONDUCTIVE STOP MEMBERS" by Dycus et al. which is hereby incorporated by reference in its entirety herein.

Jaw member **120** is designed to be fixed to the end of a rotating tube **160** which is part of the rotating assembly **80** such that rotation of the tube **160** will impart rotation to the end effector assembly **100** (See FIGS. **25** and **27**). Jaw member **120** includes a rear C-shaped cuff **170** having a slot **177** defined therein which is dimensioned to receive a slide pin **171**. More particularly, slide pin **171** includes a slide rail **176** which extends substantially the length thereof which is dimensioned to slide into friction-fit engagement within slot **177**. A pair of chamfered plates **172a** and **172b** extend generally radially from the slide rail **176** and include a radius which is substantially the same radius as the outer periphery of the rotating tube **160** such that the shaft **12** can encompass each of the same upon assembly.

As explained in more detail below, fixed jaw member **120** is connected to a second electrical potential through tube **160** which is connected at its proximal end to lead **310c**. More particularly, fixed jaw **120** is welded to the rotating tube **160** and includes a fuse clip, spring clip or other electro-mechanical connection which provides electrical continuity to the fixed jaw member **120** from lead **310c** (See FIG. **32**). As best shown in FIGS. **25** and **26**, the rotating tube **160** includes an elongated guide slot **167** disposed in an

upper portion thereof which is dimensioned to carry lead **311** therealong. The chamfered plates **172a** and **172b** also form a wire channel **175** which is dimensioned to guide the cable lead **311** from the tube **160** and into the movable jaw member **110** (See FIG. **8**). Lead **311** carries a first electrical potential to movable jaw **110**. As explained in more detail below with respect to the internal electrical connections of the forceps, a second electrical connection from lead **310c** is conducted through the tube **160** to the fixed jaw member **120**.

As shown in FIG. **25**, the distal end of the tube **160** is generally C-shaped to include two upwardly extending flanges **162a** and **162b** which define a cavity **165** for receiving the proximal end of the fixed jaw member **120** inclusive of C-shaped cuff **170** and slide pin **171** (See FIG. **27**). Preferably, the tube cavity **165** retains and secures the jaw member **120** in a friction-fit manner, however, the jaw member **120** may be welded to the tube **160** depending upon a particular purpose. Tube **160** also includes an inner cavity **169** defined therethrough which reciprocates the knife assembly **140** upon distal activation thereof and an elongated guide rail **163** which guides the knife assembly **140** during distal activation. The details with respect to the knife assembly are explained in more detail with respect to FIGS. **21–24**. The proximal end of tube **160** includes a laterally oriented slot **168** which is designed to interface with the rotating assembly **80** as described below.

FIG. **25** also shows the rotating assembly **80** which includes C-shaped rotating halves **82a** and **82b** which, when assembled about tube **160**, form a generally circular rotating member **82**. More particularly, each rotating half, e.g., **82b**, includes a series of mechanical interfaces **375a**, **375b**, **375c** and **375d** which matingly engage a corresponding series of mechanical interfaces in half **82a** to form rotating member **82**. Half **82b** also includes a tab **89b** which together with a corresponding tab **89a** disposed on half **82a** (phantomly illustrated) cooperate to matingly engage slot **168** disposed on tube **160**. As can be appreciated, this permits selective rotation of the tube **160** about axis “A” by manipulating the rotating member **82** in the direction of the arrow “B” (see FIG. **4**).

As best shown in the exploded view of FIG. **17**, jaw members **110** and **120** are pivotably mounted with respect to one another such that jaw member **110** pivots in a unilateral fashion from a first open position to a second closed position for grasping and manipulating tissue **420**. More particularly, fixed jaw member **120** includes a pair of proximal, upwardly extending flanges **125a** and **125b** which define a cavity **121** dimensioned to receive flange **118** of movable jaw member **110** therein. Each of the flanges **125a** and **125b** includes an aperture **101a** and **101b**, respectively, defined therethrough which secures pivot pin **103** on opposite sides of pivot mount **119** disposed within jaw member **110**. As explained in detail below with respect to the operation of the jaw members **110** and **120**, proximal movement of the tube **60** engages detent **117** to pivot the jaw member **110** to a closed position.

FIGS. **13** and **14** show the details of the housing **20** and the component features thereof, namely, the drive assembly **150**, the rotating assembly **80**, the knife assembly **140**, the trigger assembly **70** and the handles **40** and **50**. More particularly, FIG. **13** shows the above-identified assemblies and components in an assembled form in the housing **20** and FIG. **14** shows an exploded view of each of the above-identified assemblies and components.

As shown best in FIG. **14**, the housing includes halves **20a** and **20b** which, when mated, form housing **20**. As can be

appreciated, housing **20**, once formed, houses the various assemblies identified above which will enable a user to selectively manipulate, grasp, seal and sever tissue **420** in a simple, effective, and efficient manner. Preferably, each half of the housing, e.g., half **20b**, includes a series of mechanical interfacing component, e.g., **27a–27f** which align and/or mate with a corresponding series of mechanical interfaces (not shown) to align the two housing halves **20a** and **20b** about the inner components and assemblies. The housing halves **20a** and **20b** are then preferably sonic welded to secure the housing halves **20a** and **20b** once assembled.

As mentioned above, the movable handle **40** includes clevis **45** which forms upper flanges **45a** and **45b** which pivot about pins **29a** and **29b** to pull the reciprocating sleeve **60** along longitudinal axis “A” and force driving flange **47** against the drive assembly **150** which, in turn, closes the jaw members **110** and **120**. As mentioned above, the lower end of the movable handle **40** includes a flange **90** which has a t-shaped distal end **95** which rides within a predefined channel **51** disposed within fixed handle **50** to lock the movable handle **40** in a preset orientation relative to the fixed handle **50**. The arrangement of the upper flanges **45a** and **45b** and the pivot point of the movable handle **40** provides a distinct mechanical advantage over conventional handle assemblies due to the unique position of the pivot pins **29a** and **29b** (i.e., pivot point) relative to the longitudinal axis “A” of the driving flange **47**. In other words, by positioning the pivot pins **29a** and **29b** above the driving flange **47**, the user gains lever-like mechanical advantage to actuate the jaw members **110** and **120**. This reduces the overall amount of mechanical force necessary to close the jaw members **110** and **120** to effect a tissue seal.

Handle **40** also includes a finger loop **41** which defines opening **42** which is dimensioned to facilitate grasping the handle **40**. Preferably, finger loop **41** includes rubber insert **43** which enhances the overall ergonomic “feel” of the handle member **40**. A locking flange **44** is disposed on the outer periphery of the handle member **40** above the finger loop **41**. Locking flange **44** prevents the trigger assembly **70** from firing when the handle member **40** is oriented in a non-actuated position, i.e., the jaw members **110** and **120** are open. As can be appreciated, this prevents accidental or premature severing of tissue **420** prior to completion of the tissue seal **450**.

Fixed handle **50** includes halves **50a** and **50b** which, when assembled, form handle **50**. Fixed handle **50** includes a channel **51** defined therein which is dimensioned to receive flange **90** in a proximal moving manner when movable handle **40** is actuated. The t-shaped free end **95** of handle **40** is dimensioned for facile reception within channel **51** of handle **50**. It is envisioned that flange **90** may be dimensioned to allow a user to selectively, progressively and/or incrementally move jaw members **110** and **120** relative to one another from the open to closed positions. For example, it is also contemplated that flange **90** may include a ratchet-like interface which lockingly engages the movable handle **40** and, therefore, jaw members **110** and **120** at selective, incremental positions relative to one another depending upon a particular purpose. Other mechanisms may also be employed to control and/or limit the movement of handle **40** relative to handle **50** (and jaw members **110** and **120**) such as, e.g., hydraulic, semi-hydraulic, linear actuator(s), gas-assisted mechanisms and/or gearing systems.

As best illustrated in FIG. **13**, housing halves **20a** and **20b** when assembled form an internal cavity **52** which predefines the channel **51** within fixed handle **50** such that an entrance pathway **54** and an exit pathway **58** are formed for recip-

roca- tion of the t-shaped flange end 95 therein. When assembled, two generally triangular-shaped members 57 (one disposed in each handle half 50a and 50b) are positioned in close abutment relative to one another to define a rail or track 192 therebetween. During movement of the flange 90 along the entrance and exit pathways 54 and 58, respectively, the t-shaped end 95 rides along track 192 between the two triangular members 57 according to the particular dimensions of the triangularly-shaped members 57, which, as can be appreciated, predetermines part of the overall pivoting motion of handle 40 relative to fixed handle 50.

Once actuated, handle 40 moves in a generally arcuate fashion towards fixed handle 50 about pivot pins 29a and 29b which forces driving flange 47 proximally against the drive assembly 150 which, in turn, pulls reciprocating sleeve 60 in a generally proximal direction to close jaw member 110 relative to jaw member 120. Moreover, proximal rotation of the handle 40 causes the locking flange 44 to release, i.e., “unlock”, the trigger assembly 70 for selective actuation. This feature is shown in detail with reference to FIGS. 33, 37 and 44 and the explanation of the operation of the knife assembly 70 explained below.

The operating features and relative movements of the internal working components of the forceps 10 are shown by phantom representation in the various figures. As mentioned above, when the forceps 10 is assembled a predefined channel 52 is formed within the fixed handle 50. The channel includes entrance pathway 51 and an exit pathway 58 for reciprocation of the flange 90 and the t-shaped end 95 therein. Once assembled, the two generally triangular-shaped members 57 are positioned in close abutment relative to one another and define track 192 disposed therebetween.

As the handle 40 is squeezed and flange 90 is incorporated into channel 51 of fixed handle 50, the driving flange 47, through the mechanical advantage of the above-the-center pivot points, biases flange 154 of drive ring 159 which, in turn, compresses a spring 67 against a rear ring 156 of the drive assembly 150 (FIG. 40). As a result thereof, the rear ring 156 reciprocates sleeve 60 proximally which, in turn, closes jaw member 110 onto jaw member 120. It is envisioned that the utilization of an over-the-center pivoting mechanism will enable the user to selectively compress the coil spring 67 a specific distance which, in turn, imparts a specific pulling load on the reciprocating sleeve 60 which is converted to a rotational torque about the jaw pivot pin 103. As a result, a specific closure force can be transmitted to the opposing jaw members 110 and 120.

FIGS. 37 and 38 show the initial actuation of handle 40 towards fixed handle 50 which causes the free end 95 of flange 90 to move generally proximally and upwardly along entrance pathway 51. During movement of the flange 90 along the entrance and exit pathways 51 and 58, respectively, the t-shaped end 95 rides along track 192 between the two triangular members 57. Once the desired position for the sealing site is determined and the jaw members 110 and 120 are properly positioned, handle 40 may be compressed fully such that the t-shaped end 95 of flange 90 clears a predefined rail edge 193 located atop the triangular-shaped members 57. Once end 95 clears edge 193, releasing movement of the handle 40 and flange 90 is redirected into a catch basin 194 located at the proximal end of the triangular member 57. More particularly, upon a slight reduction in the closing pressure of handle 40 against handle 50, the handle 40 returns slightly distally towards entrance pathway 51 but is re-directed towards exit pathway 58. At this point, the release or return pressure between the handles 40 and 50

which is attributable and directly proportional to the release pressure associated with the compression of the drive assembly 150 causes the end 95 of flange 90 to settle or lock within catch basin 194. Handle 40 is now secured in position within fixed handle 50 which, in turn, locks the jaw members 110 and 120 in a closed position against the tissue 420.

As mentioned above, the jaw members 110 and 120 may be opened, closed and rotated to manipulate tissue 420 until sealing is desired. This enables the user to position and re-position the forceps 10 prior to activation and sealing. As illustrated in FIG. 4, the end effector assembly 100 is rotatable about longitudinal axis “A” through rotation of the rotating assembly 80. As explained in more detail below, it is envisioned that the unique feed path of the cable lead 311 through the rotating assembly 80, along shaft 12 and, ultimately, to the jaw member 110 enables the user to rotate the end effector assembly 100 about 180 degrees in both the clockwise and counterclockwise direction without tangling or causing undue strain on cable lead 311. Cable lead 310c is fused or clipped to the proximal end of tube 160 and is generally unaffected by rotation of the jaw members 110 and 120. As can be appreciated, this facilitates the grasping and manipulation of tissue 420.

Again as best shown in FIGS. 13 and 14, trigger assembly 70 mounts atop movable handle 40 and cooperates with the knife assembly 140 to selectively translate knife 185 through a tissue seal 450. More particularly, the trigger assembly 70 includes a finger actuator 71 and a U-shaped upwardly-extending flange 74 having legs 74a and 74b. A pivot pin 73 mounts the trigger assembly 70 between housing halves 20a and 20b for selective rotation thereof. A pair of safety tabs 76a and 76b are disposed atop finger actuator 71 and are dimensioned to abut the locking flange 44 on handle 40 when the handle 40 is disposed in a non-actuated position, i.e., the jaw members 110 and 120 are opened.

As best seen in FIG. 14, the legs 74a and 74b of the U-shaped flange 74 each include a respective slot 77a and 77b defined therein which are each dimensioned to receive a free end of an elongated drive bar 75. Drive bar 75, in turn, is dimensioned to sit within a drive slot 147 which is part of the knife assembly 140 explained in detail below. The trigger assembly 70 is mounted atop the donut-like drive ring 141 of the knife assembly 140. Proximal activation of the finger actuator 71 rotates the trigger assembly 70 about pivot pin 73 which, in turn, forces the drive bar 75 distally, which, as explained in more detail below, ultimately extends the knife 185 through the tissue 420. A spring 350 biases the knife assembly 70 in a retracted position such that after severing tissue 420 the knife 185 and the knife assembly 70 are automatically returned to a pre-firing position.

As mentioned above, the locking flange 44 abuts tabs 76a and 76b when the handle 40 is disposed in a non-actuated position. When the handle 40 is actuated and flange 90 is fully reciprocated within channel 51 of the fixed handle 50, the locking flange 44 moves proximally allowing activation of the trigger assembly 70 (See FIGS. 37 and 44).

Drive assembly 150 includes reciprocating sleeve 60, drive housing 158, spring 67, drive ring 159, drive stop 155 and guide sleeve 157 which all cooperate to form the drive assembly 150. More particularly and as best shown in FIGS. 28 and 29, the reciprocating sleeve 60 includes a distal end 65 which as mentioned above has an aperture 62 formed therein for actuating the detent 117 of jaw member 110. The distal end 65 preferably includes a scoop-like support member 69 for supporting the proximal end of the fixed jaw member 120 therein. The proximal end 61 of the reciprocating sleeve 60 includes a slot 68 defined therein which is

dimensioned to slidably support the knife assembly 70 for longitudinal reciprocation thereof to sever tissue 420. The slot 68 also permits retraction of the reciprocating sleeve 60 over the knife assembly 140 during the closing of jaw member 110 relative to jaw member 120.

The proximal end 61 of the reciprocating sleeve 60 is positioned within an aperture 151 in drive housing 158 to permit selective reciprocation thereof upon actuation of the movable handle 40. The spring 67 is assembled atop the drive housing 158 between a rear stop 156 of the drive housing 158 and a forward stop 154 of the drive ring 159 such that movement of the forward stop 154 compresses the spring 67 against the rear stop 156 which, in turn, reciprocates the drive sleeve 60. As a result thereof, the jaw members 110 and 120 and the movable handle 40 are biased by spring 67 in an open configuration. The drive stop 155 is fixedly positioned atop the drive housing 158 and biases the upper flanges 45a and 45b of the movable handle 40 when actuated such that the driving flange 47 forces the stop 154 of the drive ring 159 proximally against the force of the spring 67. The spring 67, in turn, forces the rear stop 156 proximally to reciprocate the sleeve 60 (See FIG. 40). Preferably, the rotating assembly 80 is located proximate the driving flange 47 to facilitate rotation of the end effector assembly 100. The guide sleeve 157 mates with the proximal end 61 of the reciprocating sleeve 60 and affixes to the drive housing 158. The assembled drive assembly 150 is shown best in FIG. 20.

As best shown in FIGS. 18 and 21–24, the knife assembly shaft 180 includes an elongated rod 182 having a bifurcated distal end comprising prongs 182a and 182b which cooperate to receive a knife bar 184 therein. The knife assembly shaft 180 also includes a proximal end 183 which is keyed to facilitate insertion into tube 160 of the rotating assembly 80. A knife wheel 148 is secured to the knife bar 182 by a pin 143. More particularly, the elongated knife rod 182 includes apertures 181a and 181b which are dimensioned to receive and secure the knife wheel 148 to the knife rod 182 such that longitudinal reciprocation of the knife wheel 148, in turn, moves the elongated knife rod 182 to sever tissue 420.

The knife wheel 148 is preferably donut-like and includes rings 141a and 141b which define a drive slot 147 designed to receive the drive bar 75 of the trigger assembly 70 such that proximal actuation of the trigger assembly 70 forces the drive bar 75 and the knife wheel 148 distally. It is envisioned that aperture 181a may be used for a particular trigger assembly 70 configuration and aperture 181b may be used for a different trigger assembly 70 configuration. As such, pin 143 is designed for attachment through either aperture 181a or 181b to mount the knife wheel 148 (See FIG. 24). Knife wheel 148 also includes a series of radial flanges 142a and 142b which are dimensioned to slide along both channel 163 of tube 160 and slot 68 of the reciprocating sleeve 60 (See FIG. 15).

As mentioned above, the knife rod 182 is dimensioned to mount the knife bar 184 between prongs 182a and 182b preferably in friction-fit engagement. The knife bar 184 includes a series of steps 186a, 186b and 186c which reduce the profile of the knife bar 184 towards the distal end thereof. The distal end of the knife bar 184 includes a knife support 188 which is dimensioned to retain knife blade 185. The end of the knife support preferably includes a chamfered edge 188a. It is envisioned that the knife blade 185 may be welded to the knife support 188 or secured in any manner known in the trade.

As best shown in the exploded view of the FIGS. 14 and 30–32, the electrical leads 310a, 310b, 310c and 311 are fed through the housing 20 by electro-surgical cable 310. More particularly, the electro-surgical cable 310 is fed into the bottom of the housing 20 through fixed handle 50. Lead 310c extends directly from cable 310 into the rotating assembly 80 and connects (via a fused clip or spring clip or the like) to tube 60 to conduct the second electrical potential to fixed jaw member 120. Leads 310a and 310b extend from cable 310 and connect to the hand switch or joy-stick-like toggle switch 200.

Switch 200 includes an ergonomically dimensioned toggle plate 205 having a pair of wings 207a and 207b which preferably conform to the outer shape of housing 20 (once assembled). It is envisioned that the switch 200 permits the user to selectively activate the forceps 10 in a variety of different orientations, i.e., multi-oriented activation. As can be appreciated, this simplifies activation. A pair of prongs 204a and 204b extend distally and mate with a corresponding pair of mechanical interfaces 21a and 21b disposed within housing 20 (See FIG. 32). Prongs 204a and 204b preferably snap-fit to the housing 20 during assembly. Toggle plate 205 also includes a switch interface 203 which mates with a switch button 202 which, in turn, connects to electrical interface 201. The electrical leads 310a and 310b are electrically connected to electrical interface 201. When the toggle plate 205 is depressed, trigger lead 311 carries the first electrical potential to jaw member 110. More particularly, lead 311 extends from interface 201 through a plurality of slots 84a, 84b and 84c of the rotating assembly 80 (See FIGS. 25 and 30) and along the upper portion of tube 160 and eventually connects to the movable jaw member 110 as described above (See FIGS. 32, 34 and 35).

When the switch 200 is depressed, electro-surgical energy is transferred through leads 311 and 310c to jaw members 110 and 120, respectively. It is envisioned that a safety switch or circuit (not shown) may be employed such that the switch cannot fire unless the jaw members 110 and 120 are closed and/or unless the jaw members 110 and 120 have tissue 420 held therebetween. In the latter instance, a sensor (not shown) may be employed to determine if tissue 420 is held therebetween. In addition, other sensor mechanisms may be employed which determine pre-surgical, concurrent surgical (i.e., during surgery) and/or post surgical conditions. The sensor mechanisms may also be utilized with a closed-loop feedback system coupled to the electro-surgical generator to regulate the electro-surgical energy based upon one or more pre-surgical, concurrent surgical or post surgical conditions. Various sensor mechanisms and feedback systems are described in commonly-owned, co-pending U.S. patent application Ser. No. 10/427,832 entitled “METHOD AND SYSTEM FOR CONTROLLING OUTPUT OF RF MEDICAL GENERATOR” filed on May 1, 2003 the entire contents of which are hereby incorporated by reference herein.

Preferably, the jaw members 110 and 120 are electrically isolated from one another such that electro-surgical energy can be effectively transferred through the tissue 420 to form seal 450. For example and as best illustrated in FIGS. 32, 34 and 35, each jaw member, e.g., 110, includes a uniquely-designed electro-surgical cable path disposed therethrough which transmits electro-surgical energy to the electrically conductive sealing surface 112. It is envisioned that jaw member 110 may include one or more cable guides or crimp-like electrical connectors to direct cable lead 311 towards electrically conductive sealing surface 112. Preferably, cable lead 311 is held loosely but securely along the

cable path to permit rotation of the jaw member **110** about pivot **103**. As can be appreciated, this isolates electrically conductive sealing surface **112** from the remaining operative components of the end effector assembly **100**, jaw member **120** and shaft **12**. As explained in detail above, the second electrical potential is conducted to jaw member **120** through tube **160**. The two potentials are isolated from one another by virtue of the insulative sheathing surrounding cable lead **311**.

It is contemplated that utilizing a cable feed path for cable lead **311** and by utilizing a conductive tube **160** to carry the first and second electrical potentials not only electrically isolates each jaw member **110** and **120** but also allows the jaw members **110** and **120** to pivot about pivot pin **103** without unduly straining or possibly tangling cable lead **311**. Moreover, it is envisioned that the simplicity of the electrical connections greatly facilitates the manufacturing and assembly process and assures a consistent and tight electrical connection for the transfer of energy through the tissue **420**.

As mentioned above, it is envisioned that cable leads **311** and **310c** are fed through respective halves **82a** and **82b** of the rotating assembly **80** in such a manner to allow rotation of the shaft **12** (via rotation of the rotating assembly **80**) in the clockwise or counter-clockwise direction without unduly tangling or twisting the cable leads **311** and **310c**. More particularly, each cable lead **311** and **310c** is fed through a series of conjoining slots **84a**, **84b**, **84c** and **84d** located in the two halves **82a** and **82b** of the rotating assembly **80**. Preferably each conjoining pair of slots, e.g., **84a**, **84b** and **84c**, **84d**, are large enough to permit rotation of the rotating assembly **80** without unduly straining or tangling the cable leads **311** and **310c**. The presently disclosed cable lead feed path is envisioned to allow rotation of the rotation assembly approximately 180 degrees in either direction.

Turning back to FIG. **14** which shows the exploded view of the housing **20**, rotating assembly **80**, trigger assembly **70**, movable handle **40** and fixed handle **50**, it is envisioned that all of these various component parts along with the shaft **12** and the end effector assembly **100** are assembled during the manufacturing process to form a partially and/or fully disposable forceps **10**. For example and as mentioned above, the shaft **12** and/or end effector assembly **100** may be disposable and, therefore, selectively/releasably engageable with the housing **20** and rotating assembly **80** to form a partially disposable forceps **10** and/or the entire forceps **10** may be disposable after use.

As best seen in FIG. **13**, once assembled, spring **67** is poised for compression atop drive housing **158** upon actuation of the movable handle **40**. More particularly, movement of the handle **40** about pivot pins **29a** and **29b** reciprocates the flange **90** into fixed handle **50** and forces drive flange **47** against flange **154** of drive ring **159** to compress spring **67** against the rear stop **156** to reciprocate the sleeve **60** (See FIG. **40**).

Preferably, the trigger assembly **70** is initially prevented from firing by the locking flange **44** disposed on movable handle **40** which abuts against the trigger assembly **70** prior to actuation. It is envisioned that the opposing jaw members **110** and **120** may be rotated and partially opened and closed without unlocking the trigger assembly **70** which, as can be appreciated, allows the user to grip and manipulate the tissue **420** without premature activation of the knife assembly **140**. As mentioned below, only when the t-shaped end **95** of flange **90** is completely reciprocated within channel **51** of the fixed handle **50** and seated within pre-defined catch basin **194** will the locking flange allow activation of the trigger assembly **70**. The operating features and relative movements

of these internal working components of the forceps **10** are shown by phantom representation and directional arrows and are best illustrated in FIGS. **36–49**.

FIG. **36** shows the forceps approximating tissue. As the handle **40** is squeezed and flange **90** is incorporated into channel **54** of fixed handle **50**, the drive flange **47**, through the mechanical advantage of the over the center pivot pins **29a** and **29b** is rotated generally proximally to compress spring **67**. Simultaneously, the reciprocating sleeve **60** is pulled proximally by the movement of rear ring **156** which, in turn, causes aperture **62** of sleeve **60** to proximally cam detent **117** and close the jaw member **110** relative to jaw member **120** (See FIGS. **37–40**).

It is envisioned that the mechanical advantage of the over-the-center pivot will enable the user to selectively compress the coil spring **67** a specific distance which, in turn, imparts a specific load on the reciprocating sleeve **60**. The reciprocating sleeve's **60** load is converted to a torque about the jaw pivot **103**. As a result, a specific closure force can be transmitted to the opposing jaw members **110** and **120**. As mentioned above, the jaw members **110** and **120** may be opened, closed and rotated to manipulate tissue **420** until sealing is desired without unlocking the trigger assembly **70**. This enables the user to position and re-position the forceps **10** prior to activation and sealing. More particularly, as illustrated in FIG. **4**, the end effector assembly **100** is rotatable about longitudinal axis "A" through rotation of the rotating assembly **80**.

Once the desired position for the sealing site is determined and the jaw members **110** and **120** are properly positioned, handle **40** may be compressed fully such that the t-shaped end **95** of flange **90** clears a predefined rail edge **193** located atop the triangular-shaped members **57**. Once end **95** clears edge **193**, the end is directed into catch basin **194** located within the exit pathway **58**. More particularly, upon a slight reduction in the closing pressure of handle **40** against handle **50**, the handle **40** returns slightly distally towards entrance pathway **54** but is re-directed towards exit pathway **58** into catch basin **194** (See FIG. **38**). At this point, the release or return pressure between the handles **40** and **50** which is attributable and directly proportional to the release pressure associated with the compression of the drive assembly **150** causes the end **95** of flange **90** to settle or lock within catch basin **194**. Handle **40** is now secured in position within fixed handle **50** which, in turn, locks the jaw members **110** and **120** in a closed position against the tissue **420**.

At this point the jaws members **110** and **120** are fully compressed about the tissue **420** (FIG. **26**). Moreover, the forceps **10** is now ready for selective application of electro-surgical energy and subsequent separation of the tissue **420**, i.e., as t-shaped end **95** seats within catch basin **194**, locking flange **44** moves into a position to permit activation of the trigger assembly **70** (FIGS. **44** and **45**).

As the t-shaped end **95** of flange **90** becomes seated within catch basin **194**, a proportional axial force on the reciprocating sleeve **60** is maintained which, in turn, maintains a compressive force between opposing jaw members **110** and **120** against the tissue **420**. It is envisioned that the end effector assembly **100** and/or the jaw members **110** and **120** may be dimensioned to off-load some of the excessive clamping forces to prevent mechanical failure of certain internal operating elements of the end effector **100**.

As can be appreciated, the combination of the mechanical advantage of the over-the-center pivot along with the compressive force associated with the compression spring **67** facilitate and assure consistent, uniform and accurate closure pressure about the tissue **420** within the desired working

pressure range of about 3 kg/cm² to about 16 kg/cm² and, preferably, about 7 kg/cm² to about 13 kg/cm². By controlling the intensity, frequency and duration of the electrosurgical energy applied to the tissue **420**, the user can either cauterize, coagulate/desiccate, seal and/or simply reduce or slow bleeding. As mentioned above, two mechanical factors play an important role in determining the resulting thickness of the sealed tissue and effectiveness of the seal **450**, i.e., the pressure applied between opposing jaw members **110** and **120** and the gap distance “G” between the opposing sealing surfaces **112**, **122** of the jaw members **110** and **120** during the sealing process. However, thickness of the resulting tissue seal **450** cannot be adequately controlled by force alone. In other words, too much force and the two jaw members **110** and **120** would touch and possibly short resulting in little energy traveling through the tissue **420** thus resulting in a bad tissue seal **450**. Too little force and the seal **450** would be too thick.

Applying the correct force is also important for other reasons: to oppose the walls of the vessel; to reduce the tissue impedance to a low enough value that allows enough current through the tissue **420**; and to overcome the forces of expansion during tissue heating in addition to contributing towards creating the required end tissue thickness which is an indication of a good seal **450**.

Preferably, the electrically conductive sealing surfaces **112**, **122** of the jaw members **110**, **120**, respectively, are relatively flat to avoid current concentrations at sharp edges and to avoid arcing between high points. In addition and due to the reaction force of the tissue **420** when engaged, jaw members **110** and **120** are preferably manufactured to resist bending. For example, the jaw members **110** and **120** may be tapered along the width thereof which is advantageous for two reasons: 1) the taper will apply constant pressure for a constant tissue thickness at parallel; 2) the thicker proximal portion of the jaw members **110** and **120** will resist bending due to the reaction force of the tissue **420**.

As mentioned above, at least one jaw member, e.g., **120**, may include a stop member **750** which limits the movement of the two opposing jaw members **110** and **120** relative to one another. Preferably, the stop member **750** extends from the sealing surface **122** a predetermined distance according to the specific material properties (e.g., compressive strength, thermal expansion, etc.) to yield a consistent and accurate gap distance “G” during sealing (FIG. **41**). Preferably, the gap distance between opposing sealing surfaces **112** and **122** during sealing ranges from about 0.001 inches to about 0.006 inches and, more preferably, between about 0.002 and about 0.003 inches. Preferably, the non-conductive stop members **750** are molded onto the jaw members **110** and **120** (e.g., overmolding, injection molding, etc.), stamped onto the jaw members **110** and **120** or deposited (e.g., deposition) onto the jaw members **110** and **120**. For example, one technique involves thermally spraying a ceramic material onto the surface of the jaw member **110** and **120** to form the stop members **750**. Several thermal spraying techniques are contemplated which involve depositing a broad range of heat resistant and insulative materials on various surfaces to create stop members **750** for controlling the gap distance between electrically conductive surfaces **112** and **122**.

As energy is being selectively transferred to the end effector assembly **100**, across the jaw members **110** and **120** and through the tissue **420**, a tissue seal **450** forms isolating two tissue halves **420a** and **420b**. At this point and with other known vessel sealing instruments, the user must remove and replace the forceps **10** with a cutting instrument (not shown)

to divide the tissue halves **420a** and **420b** along the tissue seal **450**. As can be appreciated, this is both time consuming and tedious and may result in inaccurate tissue division across the tissue seal **450** due to misalignment or misplacement of the cutting instrument along the ideal tissue cutting plane.

As explained in detail above, the present disclosure incorporates knife assembly **140** which, when activated via the trigger assembly **70**, progressively and selectively divides the tissue **420** along an ideal tissue plane in precise manner to effectively and reliably divide the tissue **420** into two sealed halves **420a** and **420b** (See FIG. **46**) with a tissue gap **475** therebetween. The knife assembly **140** allows the user to quickly separate the tissue **420** immediately after sealing without substituting a cutting instrument through a cannula or trocar port. As can be appreciated, accurate sealing and dividing of tissue **420** is accomplished with the same forceps **10**.

It is envisioned that knife blade **185** may also be coupled to the same or an alternative electrosurgical energy source to facilitate separation of the tissue **420** along the tissue seal **450** (Not shown). Moreover, it is envisioned that the angle of the knife blade tip **185** may be dimensioned to provide more or less aggressive cutting angles depending upon a particular purpose. For example, the knife blade **185** may be positioned at an angle which reduces “tissue wisps” associated with cutting. Moreover, the knife blade **185** may be designed having different blade geometries such as serrated, notched, perforated, hollow, concave, convex etc. depending upon a particular purpose or to achieve a particular result.

Once the tissue **420** is divided into tissue halves **420a** and **420b**, the jaw members **110** and **120** may be opened by re-grasping the handle **40** as explained below. It is envisioned that the knife assembly **140** generally cuts in a progressive, uni-directional fashion (i.e., distally).

As best shown in FIGS. **47–49**, re-initiation or re-grasping of the handle **40** again moves t-shaped end **95** of flange **90** generally proximally along exit pathway **58** until end **95** clears a lip **196** disposed atop triangular-shaped members **57** along exit pathway **58**. Once lip **196** is sufficiently cleared, handle **40** and flange **90** are fully and freely releasable from handle **50** along exit pathway **58** upon the reduction of grasping/gripping pressure which, in turn, returns the jaw members **110** and **120** to the open, pre-activated position.

FIGS. **50A–50C** show various view of an alternate embodiment of the knife assembly **540** and trigger assembly **570** for use with the forceps according to the present invention. More particularly, the trigger assembly **570** mounts atop movable handle **40** and cooperates with the knife assembly **540** to selectively translate knife **185** through a tissue seal **450** as described above.

The trigger assembly **570** includes a finger actuator **571** and a generally U-shaped upwardly-extending flange **574** having generally C-shaped legs **577a** and **577b**. **577a** and **577b**. Much like the aforescribed embodiment, the knife assembly **540** includes a generally donut-shaped knife collar **540** having two rings, namely, ring **541a** and **541b**. A pivot pin **573** mounts the trigger assembly **570** between housing halves **20a** and **20b** for selective rotation thereof.

The C-shaped legs **577a** and **577b** of the U-shaped flange **574** are configured to rotate about a proximally oriented imaginary pivot point **580** upon activation of the trigger assembly **570** to urge the rings **541a** and **541b** of the knife collar **541** distally. In contrast to the previously described embodiment, the legs **577a** and **577b** are configured to abut the proximal portion of ring **541a** and do not cooperate with a pin **73** to advance the knife collar **541**. Proximal activation

of the finger actuator **571** rotates the trigger assembly **570** about pivot pin **573** in the direction “CC” which, in turn, cams the legs **577a** and **577b** of the flange **574** about imaginary pivot point **580** in the direction “AA” which, in turn, forces the knife collar **541** distally in the direction “BB”. As explained in detail above, distal movement of the knife collar **541** ultimately extends the knife **185** through the tissue **420**. Spring **350** biases the knife collar **541** in a retracted position such that after severing tissue **420** the knife **185**, knife collar **541** and trigger assembly **570** are automatically returned to a pre-firing position.

It is envisioned that this particular knife assembly **540** and trigger assembly **170** arrangement provides a longer knife stroke than the aforescribed embodiment which enables the knife **185** to be further actuated for particular tissue types. In addition, it is contemplated that this particular arrangement simplifies manufacturing and assembly.

It is envisioned that the radius of curvature “r” of the C-shaped legs **577a** and **577b** of the flange **574** may be dimensioned for particular purposes, i.e., to provide different radiuses for different preferred stroke lengths which may be dependent upon tissue type and/or particular type of surgery. Moreover and as can be appreciated, the aforescribed locking flange **44** which abuts tabs **76a** and **76b** of the previously described embodiment when the handle **40** is disposed in a non-actuated position, would have to be reconfigured to accomplish a similar purpose.

From the foregoing and with reference to the various figure drawings, those skilled in the art will appreciate that certain modifications can also be made to the present disclosure without departing from the scope of the same. For example, it may be preferable to add other features to the forceps **10**, e.g., an articulating assembly to axially displace the end effector assembly **100** relative to the elongated shaft **12**.

It is also contemplated that the forceps **10** (and/or the electro-surgical generator used in connection with the forceps **10**) may include a sensor or feedback mechanism (not shown) which automatically selects the appropriate amount of electro-surgical energy to effectively seal the particularly-sized tissue grasped between the jaw members **110** and **120**. The sensor or feedback mechanism may also measure the impedance across the tissue during sealing and provide an indicator (visual and/or audible) that an effective seal has been created between the jaw members **110** and **120**. Examples of such sensor systems are described in commonly-owned U.S. patent application Ser. No. 10/427,832 entitled “METHOD AND SYSTEM FOR CONTROLLING OUTPUT OF RF MEDICAL GENERATOR” filed on May 1, 2003 the entire contents of which are hereby incorporated by reference herein.

Moreover, it is contemplated that the trigger assembly **70** may include other types of recoil mechanism which are designed to accomplish the same purpose, e.g., gas-actuated recoil, electrically-actuated recoil (i.e., solenoid), etc. It is also envisioned that the forceps **10** may be used to cut tissue **420** without sealing. Alternatively, the knife assembly **70** may be coupled to the same or alternate electro-surgical energy source to facilitate cutting of the tissue **420**.

Although the figures depict the forceps **10** manipulating an isolated vessel **420**, it is contemplated that the forceps **10** may be used with non-isolated vessels as well. Other cutting mechanisms are also contemplated to cut tissue **420** along the ideal tissue plane.

It is envisioned that the outer surface of the end effector assembly **100** may include a nickel-based material, coating, stamping, metal injection molding which is designed to

reduce adhesion between the jaw members **110** and **120** with the surrounding tissue during activation and sealing. Moreover, it is also contemplated that the conductive surfaces **112** and **122** of the jaw members **110** and **120** may be manufactured from one (or a combination of one or more) of the following materials: nickel-chrome, chromium nitride, Med-Coat 2000 manufactured by The Electrolyzing Corporation of OHIO, inconel 600 and tin-nickel. The tissue conductive surfaces **112** and **122** may also be coated with one or more of the above materials to achieve the same result, i.e., a “non-stick surface”. As can be appreciated, reducing the amount that the tissue “sticks” during sealing improves the overall efficacy of the instrument.

One particular class of materials disclosed herein has demonstrated superior non-stick properties and, in some instances, superior seal quality. For example, nitride coatings which include, but are not limited to: TiN, ZrN, TiAlN, and CrN are preferred materials used for non-stick purposes. CrN has been found to be particularly useful for non-stick purposes due to its overall surface properties and optimal performance. Other classes of materials have also been found to reducing overall sticking. For example, high nickel/chrome alloys with a Ni/Cr ratio of approximately 5:1 have been found to significantly reduce sticking in bipolar instrumentation. One particularly useful non-stick material in this class is Inconel 600. Bipolar instrumentation having sealing surfaces **112** and **122** made from or coated with Ni200, Ni201 (~100% Ni) also showed improved non-stick performance over typical bipolar stainless steel electrodes.

As can be appreciated, locating the switch **200** on the forceps **10** has many advantages. For example, the switch **200** reduces the amount of electrical cable in the operating room and eliminates the possibility of activating the wrong instrument during a surgical procedure due to “line-of-sight” activation. Moreover, decommissioning the switch **200** when the trigger is actuated eliminates unintentionally activating the device during the cutting process. It is also envisioned that the switch **200** may be disposed on another part of the forceps **10**, e.g., the fixed handle **40**, rotating assembly **80**, housing **20**, etc.

It is further envisioned by the present disclosure for a forceps **600** to include a safety mechanism **610** disposed at least partially within housing **20** for releasably locking trigger assembly **70**, as shown in FIGS. **51** and **52**. Safety mechanism **610** is configured to link trigger assembly **70** with handle member **40**, such that when the handle member **40** is actuated (FIG. **52**), the trigger assembly **70** is released from its safety position within housing **20**. Accordingly, safety mechanism **600** prevents the trigger assembly **70** from firing when the handle member **40** is oriented in a non-actuated position (FIG. **51**), i.e., the jaw members **110** and **120** are open. As can be appreciated, this prevents accidental or premature severing of tissue **420** prior to completion of the tissue seal **450**.

While several embodiments of the disclosure have been shown in the drawings, it is not intended that the disclosure be limited thereto, as it is intended that the disclosure be as broad in scope as the art will allow and that the specification be read likewise. Therefore, the above description should not be construed as limiting, but merely as exemplifications of preferred embodiments. Those skilled in the art will envision other modifications within the scope and spirit of the claims appended hereto.

What is claimed is:

1. An endoscopic bipolar forceps, comprising: a shaft having a movable jaw member and a fixed jaw member at a distal end thereof;

25

a drive assembly for moving the movable jaw member relative to the fixed jaw member from a first position wherein the movable jaw member is disposed in spaced relation relative to the fixed jaw member to a second position wherein the movable jaw member is closer to the fixed jaw member for manipulating tissue; 5

a movable handle for actuating the drive assembly to move the movable jaw member;

each jaw member adapted to connect to a source of electrical energy such that the jaw members are capable of conducting energy through tissue held therebetween to effect a tissue seal; 10

a trigger assembly operatively disposed relative to the movable handle for selectively advancing a knife assembly for cutting tissue along the tissue seal, the knife assembly including a generally donut-shaped collar which cooperates with a knife shaft to advance a knife through tissue upon activation of the trigger assembly, the trigger assembly including a trigger and 15

26

a flange having two C-shaped legs which are configured to abut a proximal end of the knife collar such that rotation of the trigger, in turn, rotates the C-shaped legs and urges the knife collar distally to advance the knife through tissue.

2. An endoscopic bipolar forceps according to claim 1 further comprising a spring for biasing the knife collar and the trigger assembly in a proximal, unactuated position.

3. An endoscopic bipolar forceps according to claim 1 wherein a radius of curvature of the C-shaped legs of the flange is dimensioned to provide a particular stroke length of the knife.

4. An endoscopic bipolar forceps according to claim 1 further comprising a safety mechanism disposed relative to the movable handle for releasably locking the trigger assembly.

* * * * *