



US007170601B2

(12) **United States Patent**
Matsuda

(10) **Patent No.:** **US 7,170,601 B2**
(45) **Date of Patent:** **Jan. 30, 2007**

(54) **FLOW CELL, AND PARTICLE MEASUREMENT DEVICE USING THE SAME**

(75) Inventor: **Tomonobu Matsuda**, Tokyo (JP)

(73) Assignee: **Rion Co., Ltd.**, Tokyo (JP)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

4,276,475 A *	6/1981	Nelson	250/373
4,906,094 A *	3/1990	Ashida	356/336
5,371,585 A *	12/1994	Morgan et al.	356/246
5,506,673 A *	4/1996	Kosaka et al.	356/72
5,601,983 A *	2/1997	Takayama et al.	435/6
5,633,503 A *	5/1997	Kosaka	250/458.1
6,118,536 A *	9/2000	Sakamoto et al.	356/364
6,184,983 B1 *	2/2001	Yamaguchi et al.	356/335
6,465,802 B1 *	10/2002	Matsuda	250/574

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **10/528,900**

JP 11-211650 8/1999

(22) PCT Filed: **Sep. 27, 2002**

JP 11-211651 8/1999

(86) PCT No.: **PCT/JP02/10104**

* cited by examiner

§ 371 (c)(1),
(2), (4) Date: **Mar. 23, 2005**

Primary Examiner—Gregory J. Toatley, Jr.

Assistant Examiner—Sang H. Nguyen

(87) PCT Pub. No.: **WO2004/029589**

(74) *Attorney, Agent, or Firm*—Carrier, Blackman & Associates, P.C.; Joseph P. Carrier; William D. Blackman

PCT Pub. Date: **Apr. 8, 2004**

(57) **ABSTRACT**

(65) **Prior Publication Data**

US 2006/0001874 A1 Jan. 5, 2006

(51) **Int. Cl.**
G01N 21/00 (2006.01)

(52) **U.S. Cl.** **356/336; 356/337**

(58) **Field of Classification Search** **356/335–343, 356/440, 442, 434, 436; 250/574–575, 222.2, 250/573, 576; 435/6, 7.1, 7.9**

See application file for complete search history.

A flow cell is provided which can detect scattered light more efficiently by fully utilizing the condensing angle of a condenser lens. A particle monitoring area M is formed within the flow cell by irradiating the area with laser light La, and scattered light Ls generated by particles contained in sample fluid passing through the particle monitoring area M is condensed by the condenser lens L so as to obtain information including diameter of the particles, and inner walls of the flow cell are shaped or arranged such that the scattered light Ls is condensed in a state where the condensing angle θ of the condenser lens L is fully utilized.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,710,933 A * 1/1973 Fulwyler et al. 209/3.1

20 Claims, 4 Drawing Sheets

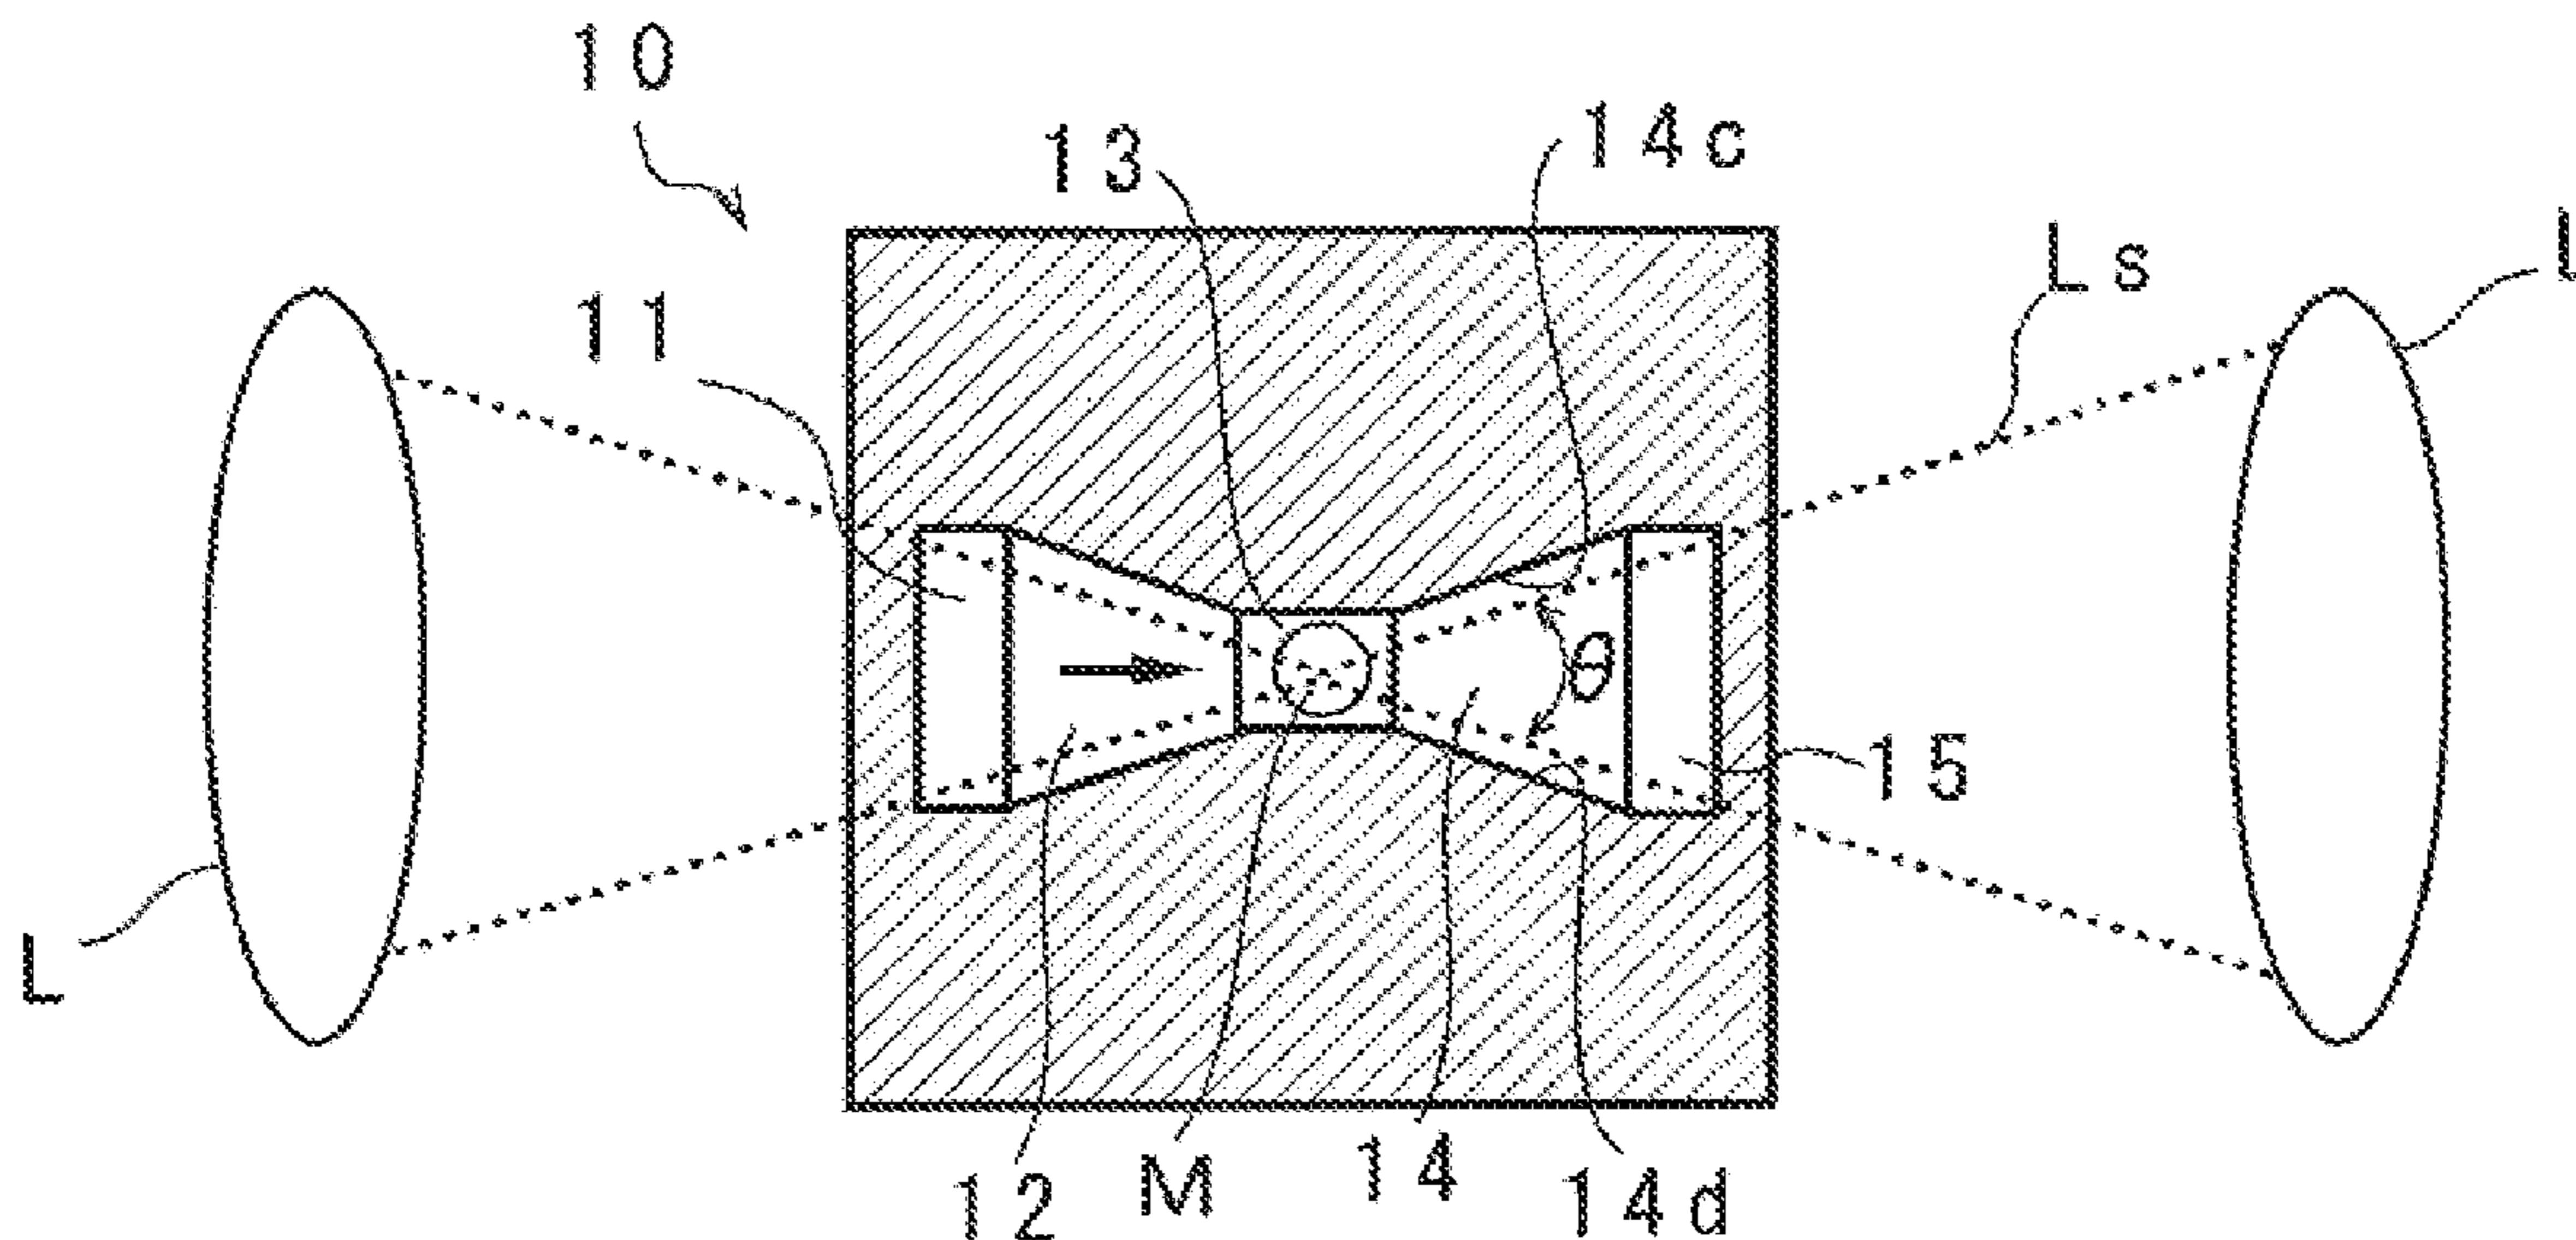


FIG. 1

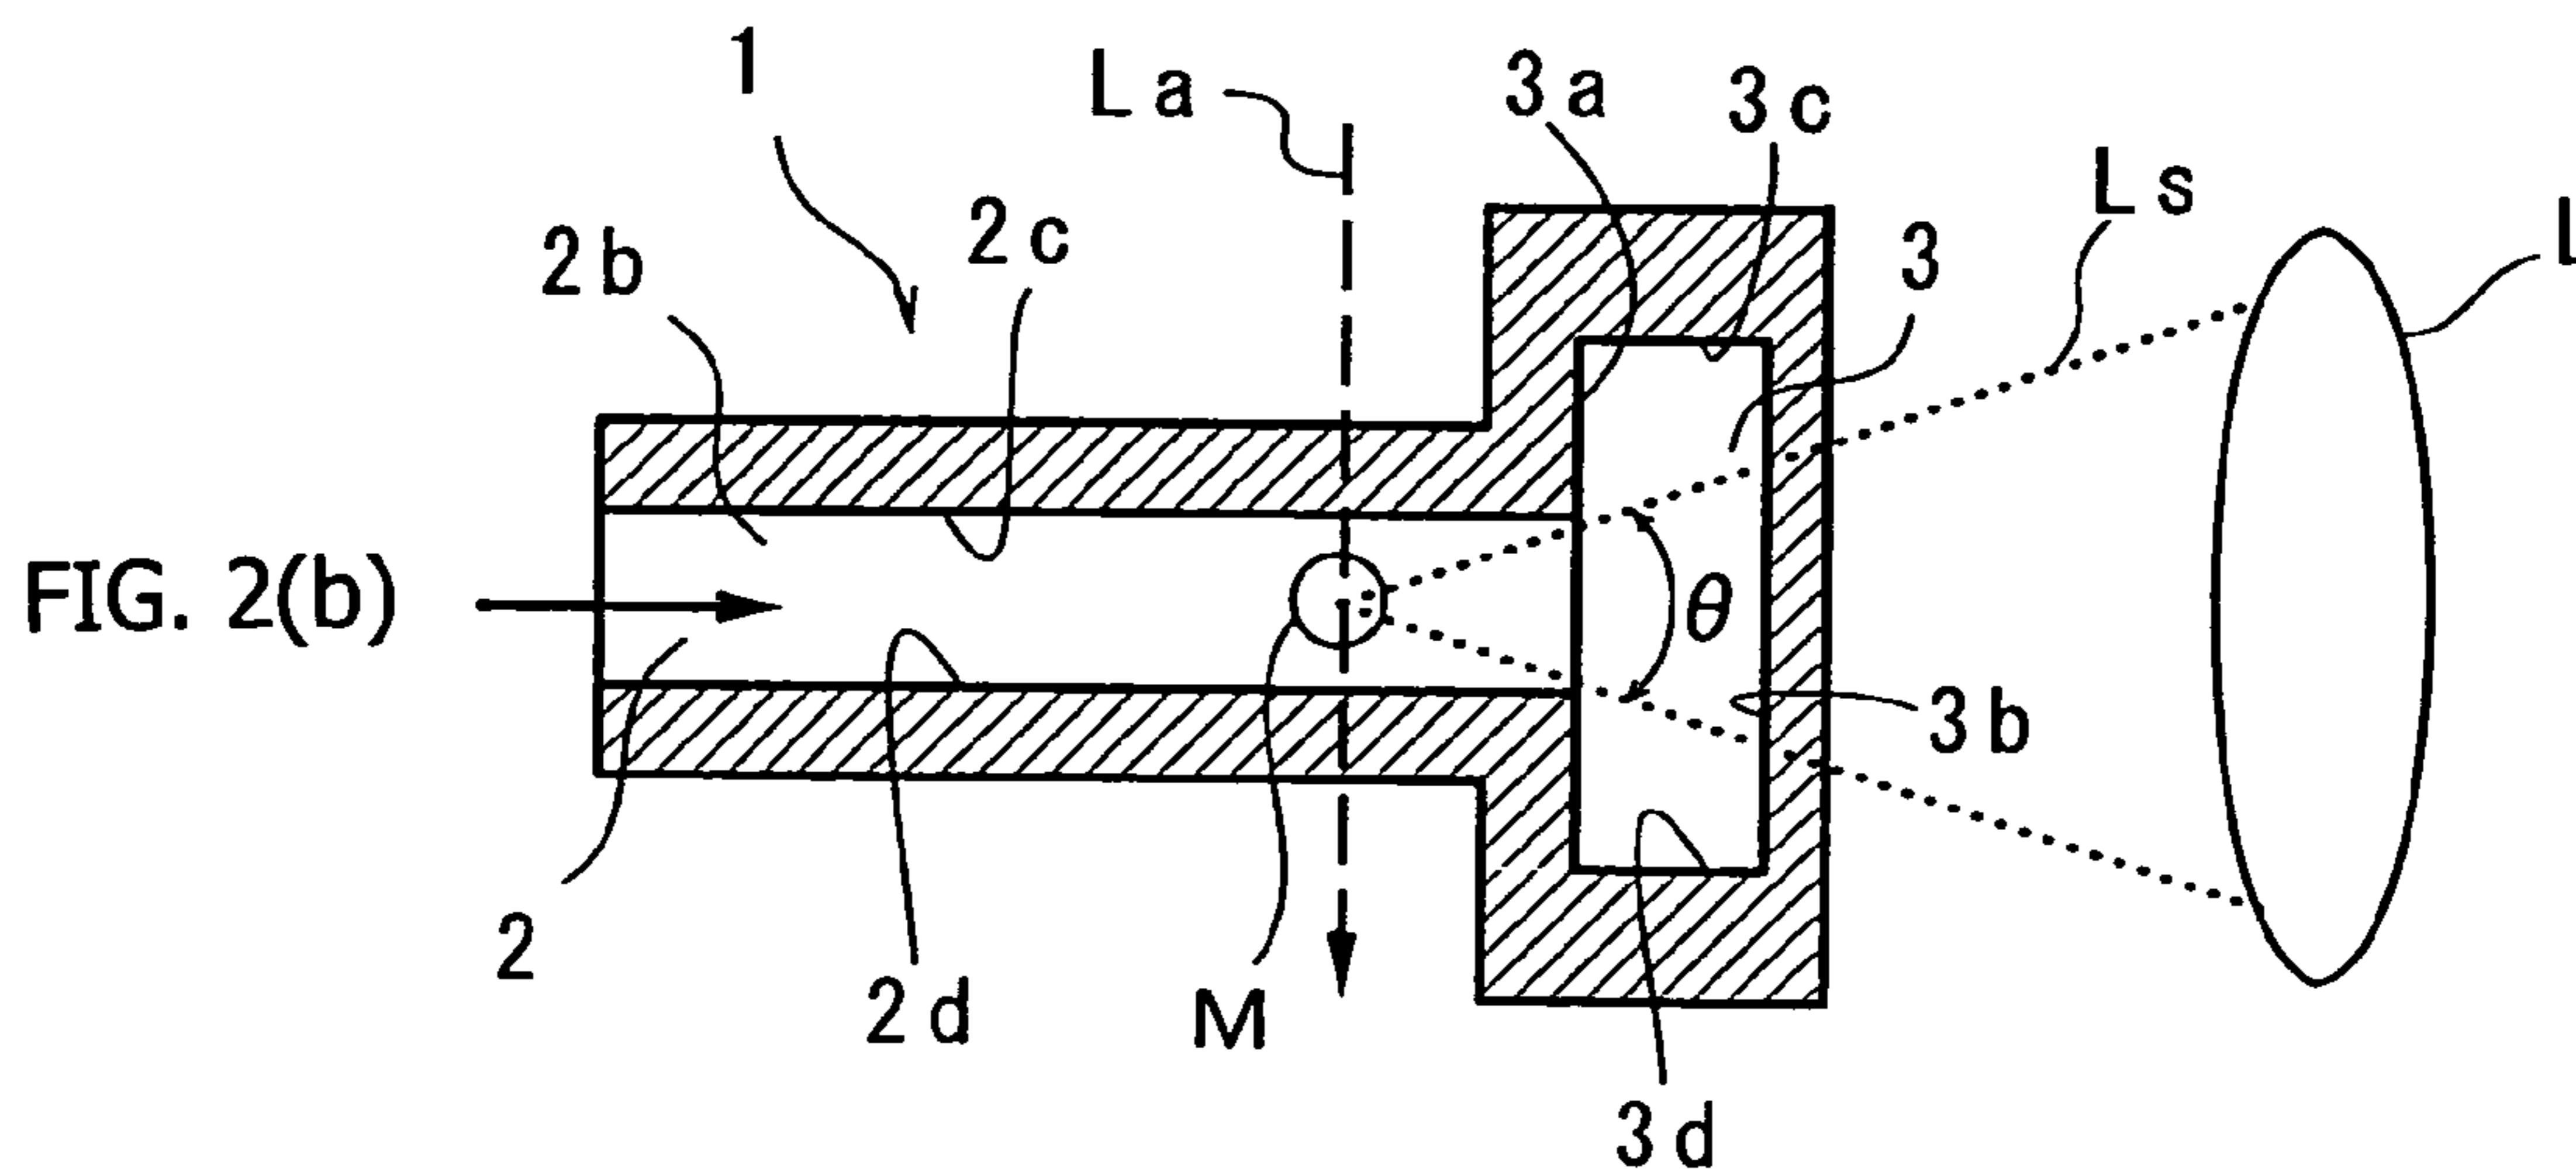
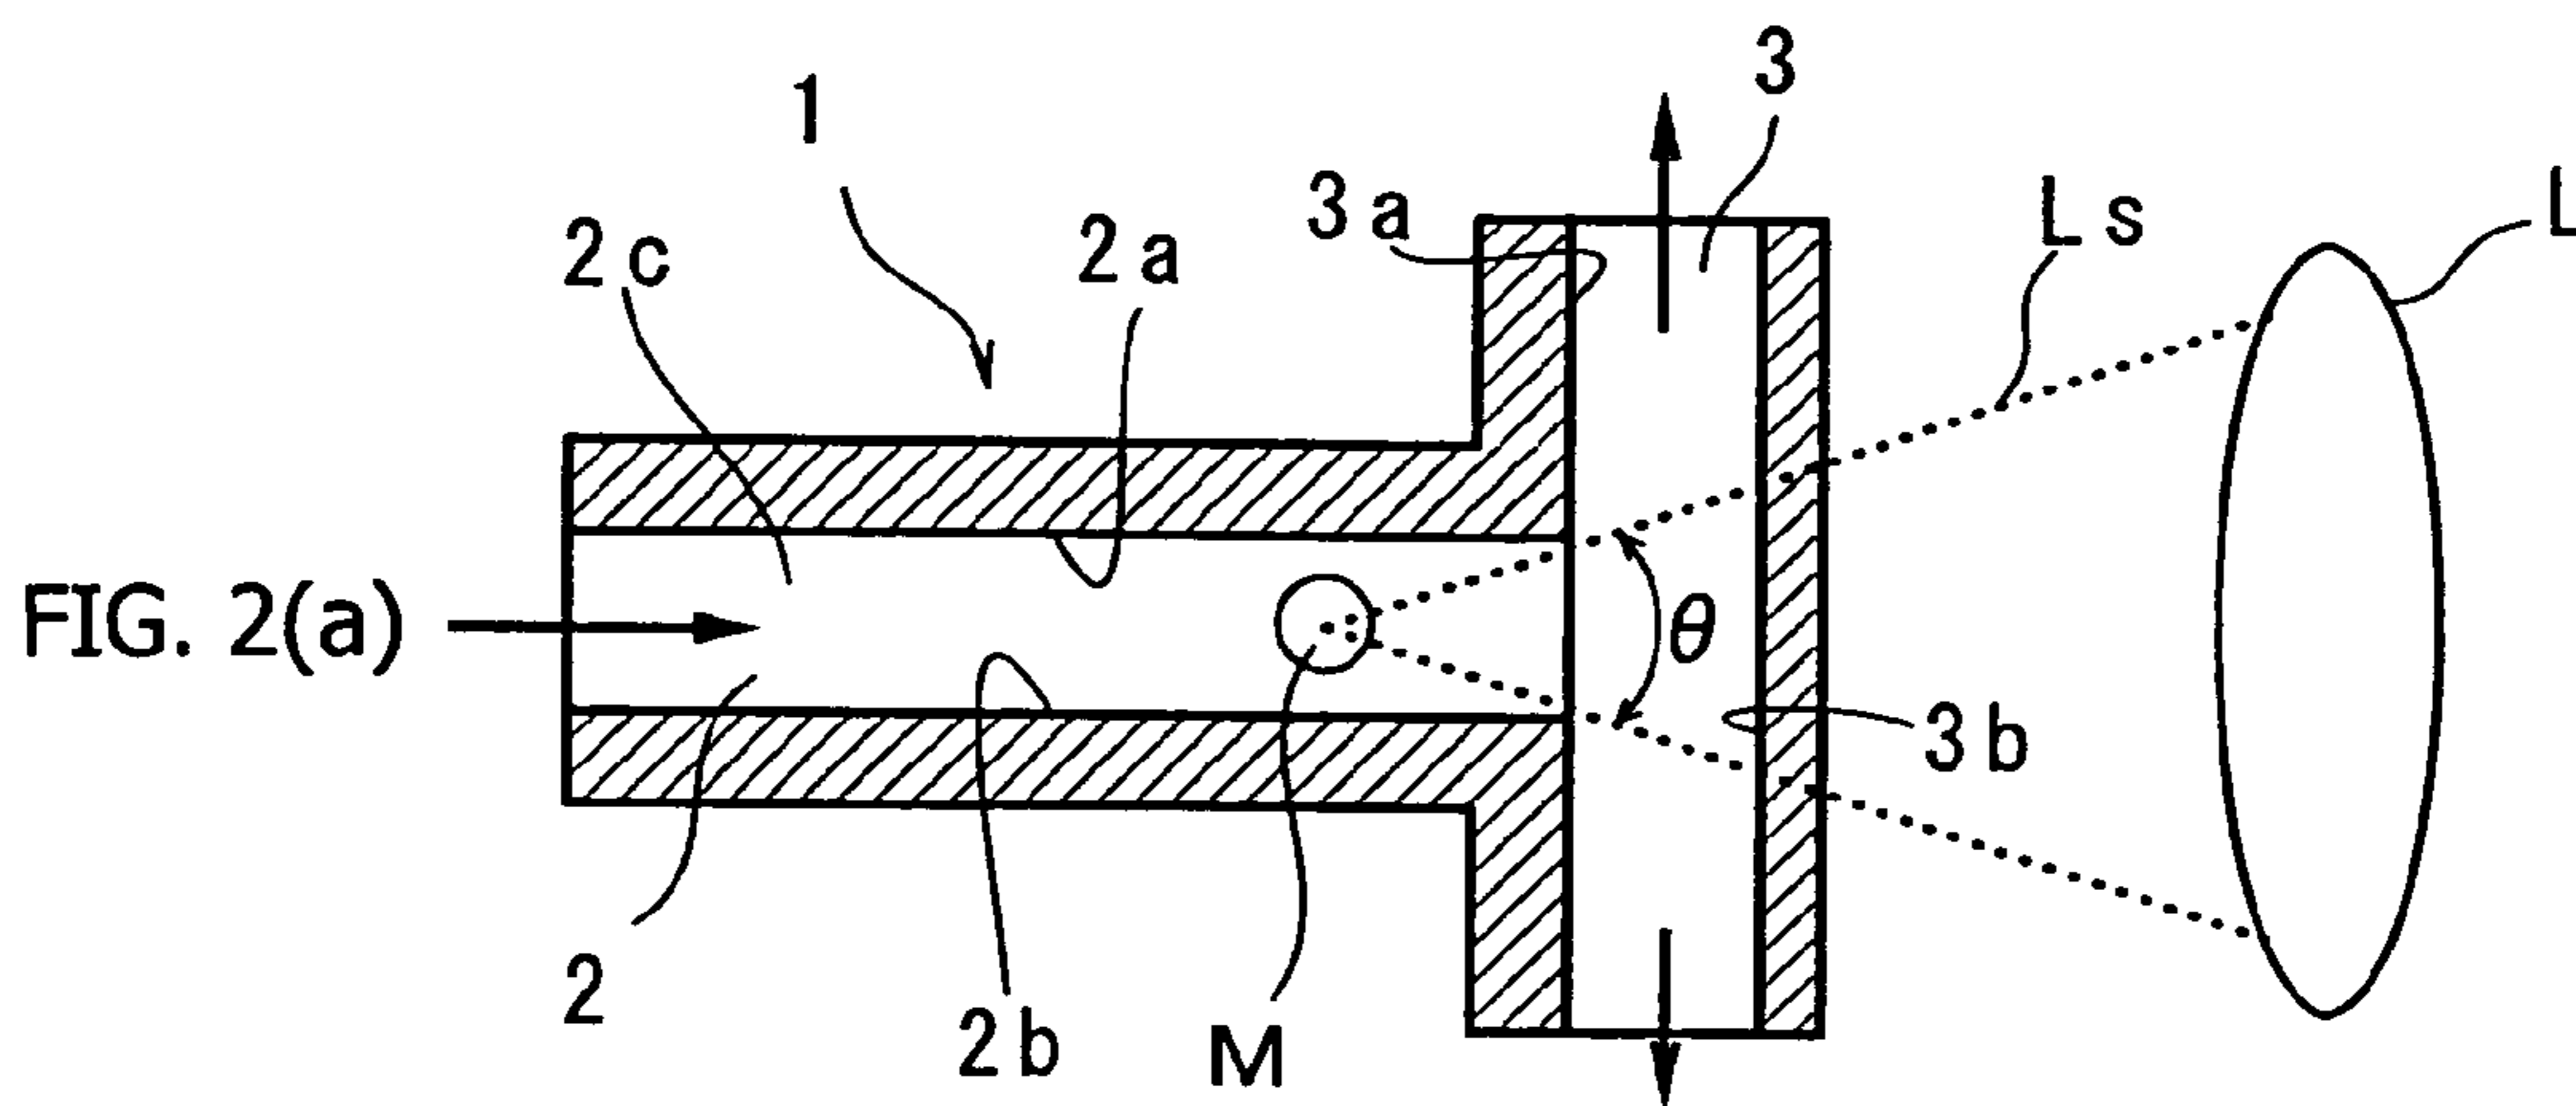
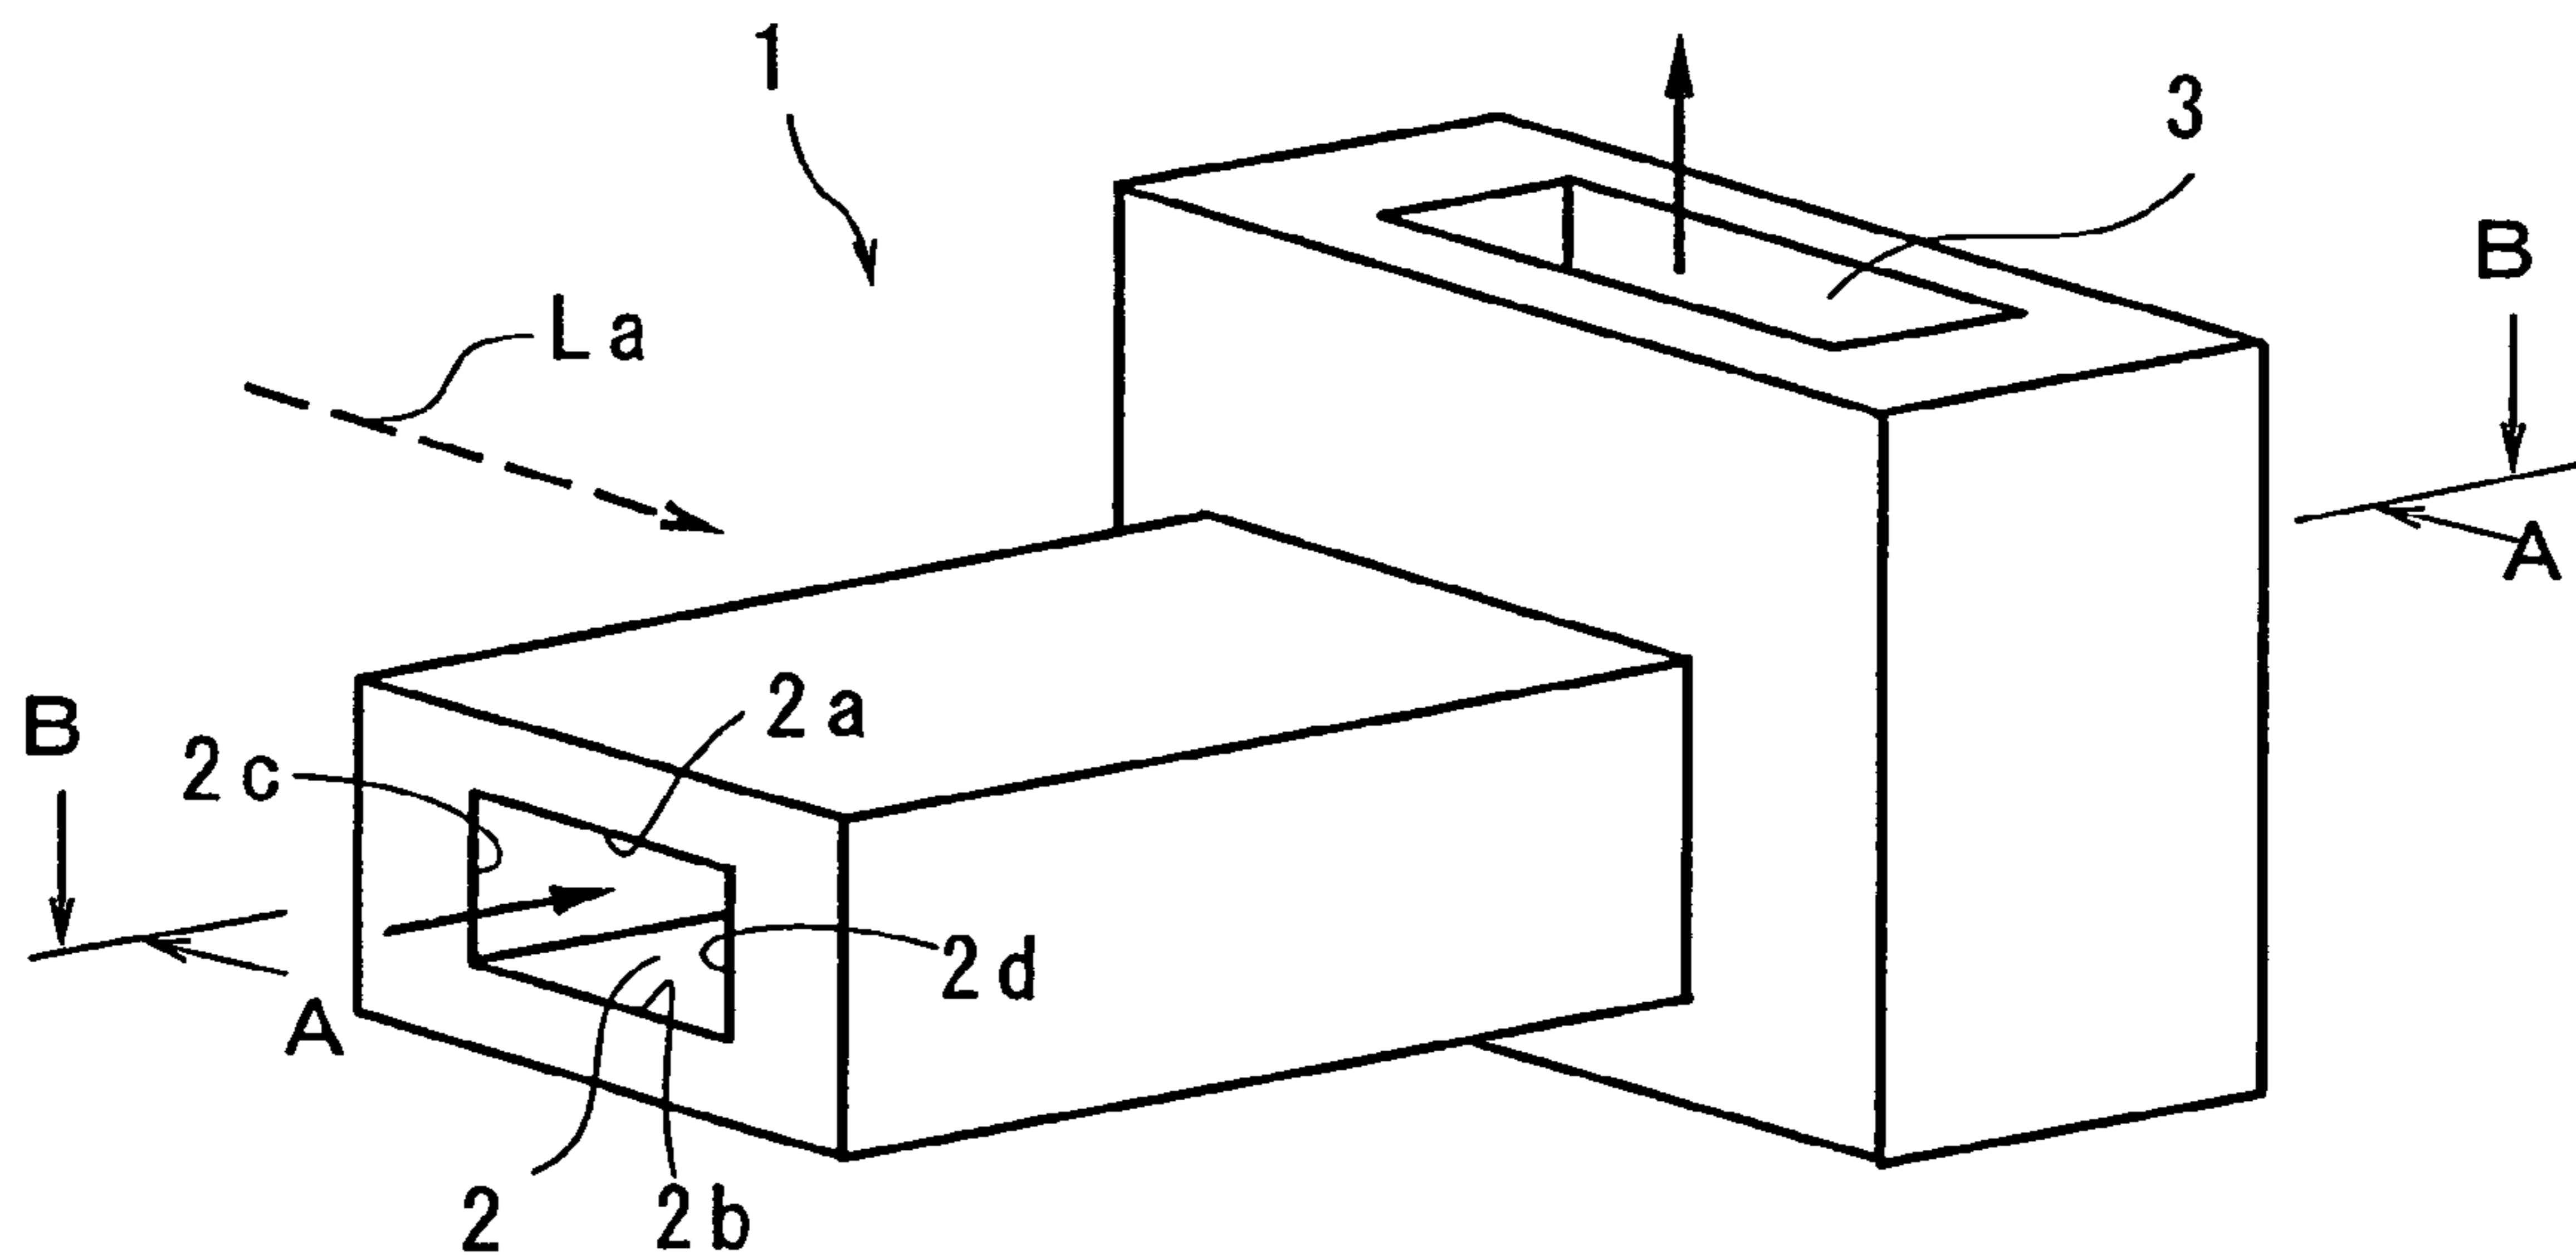


FIG. 3

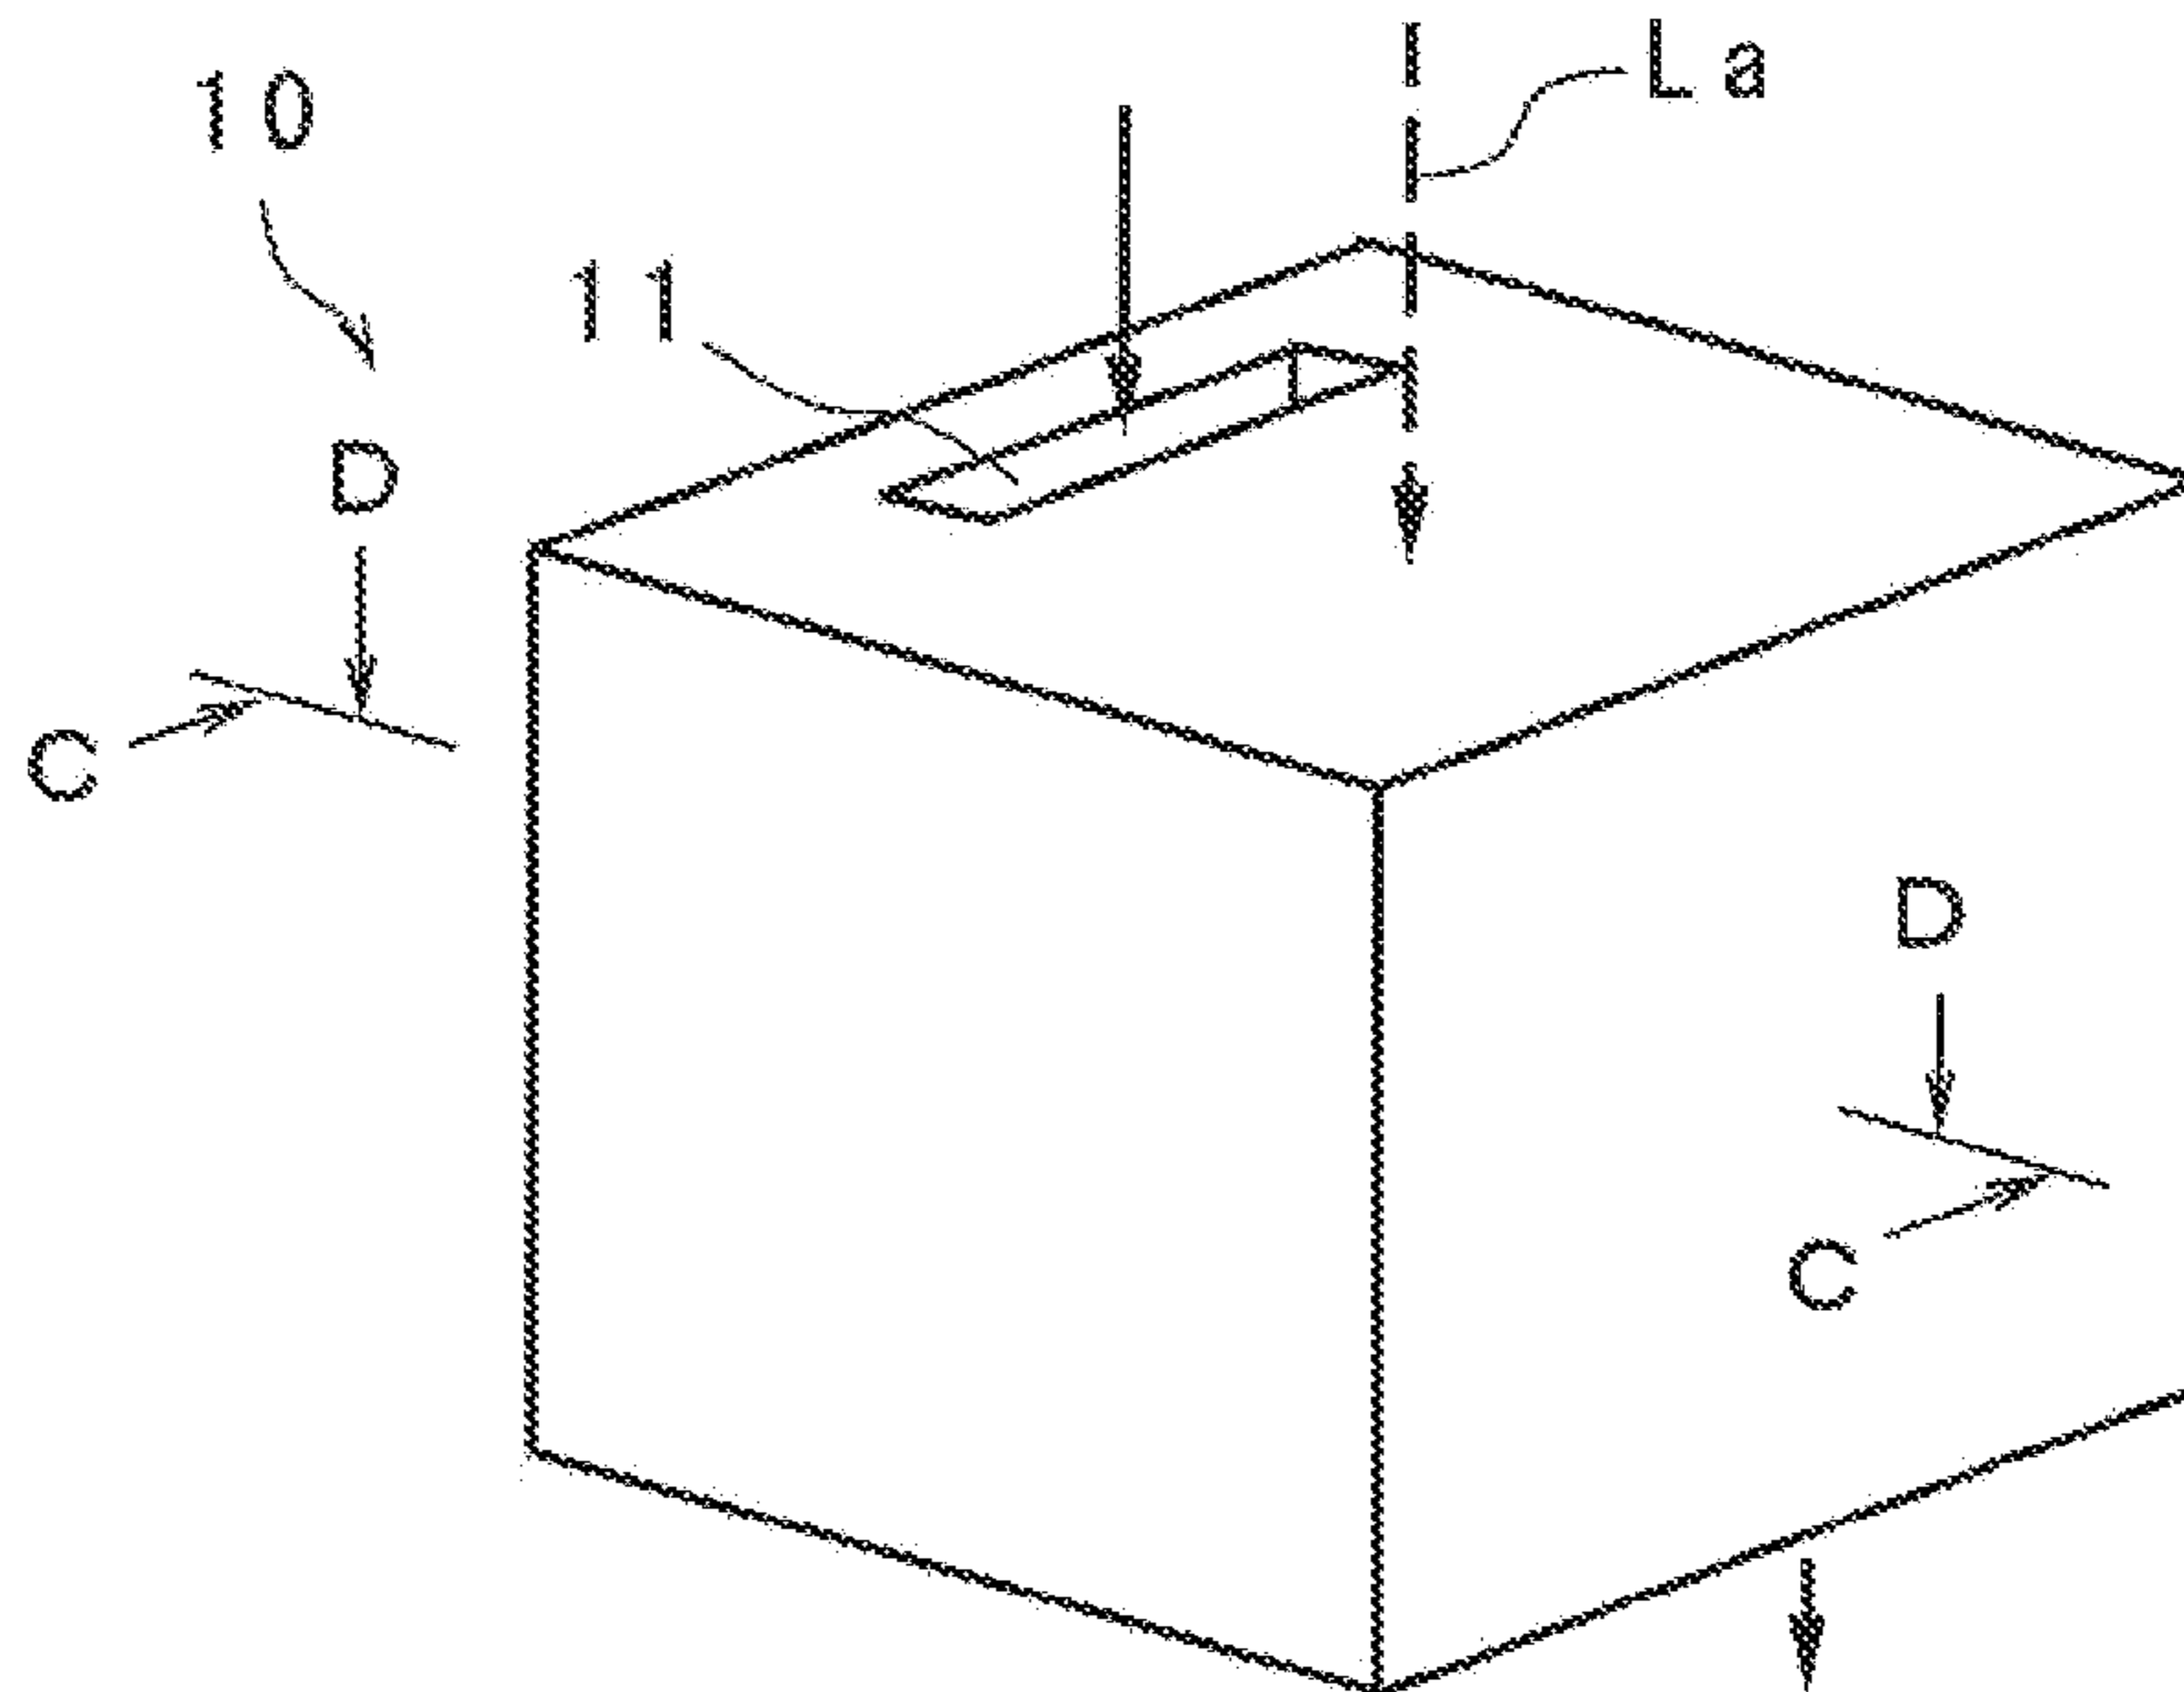


FIG. 4 (a)

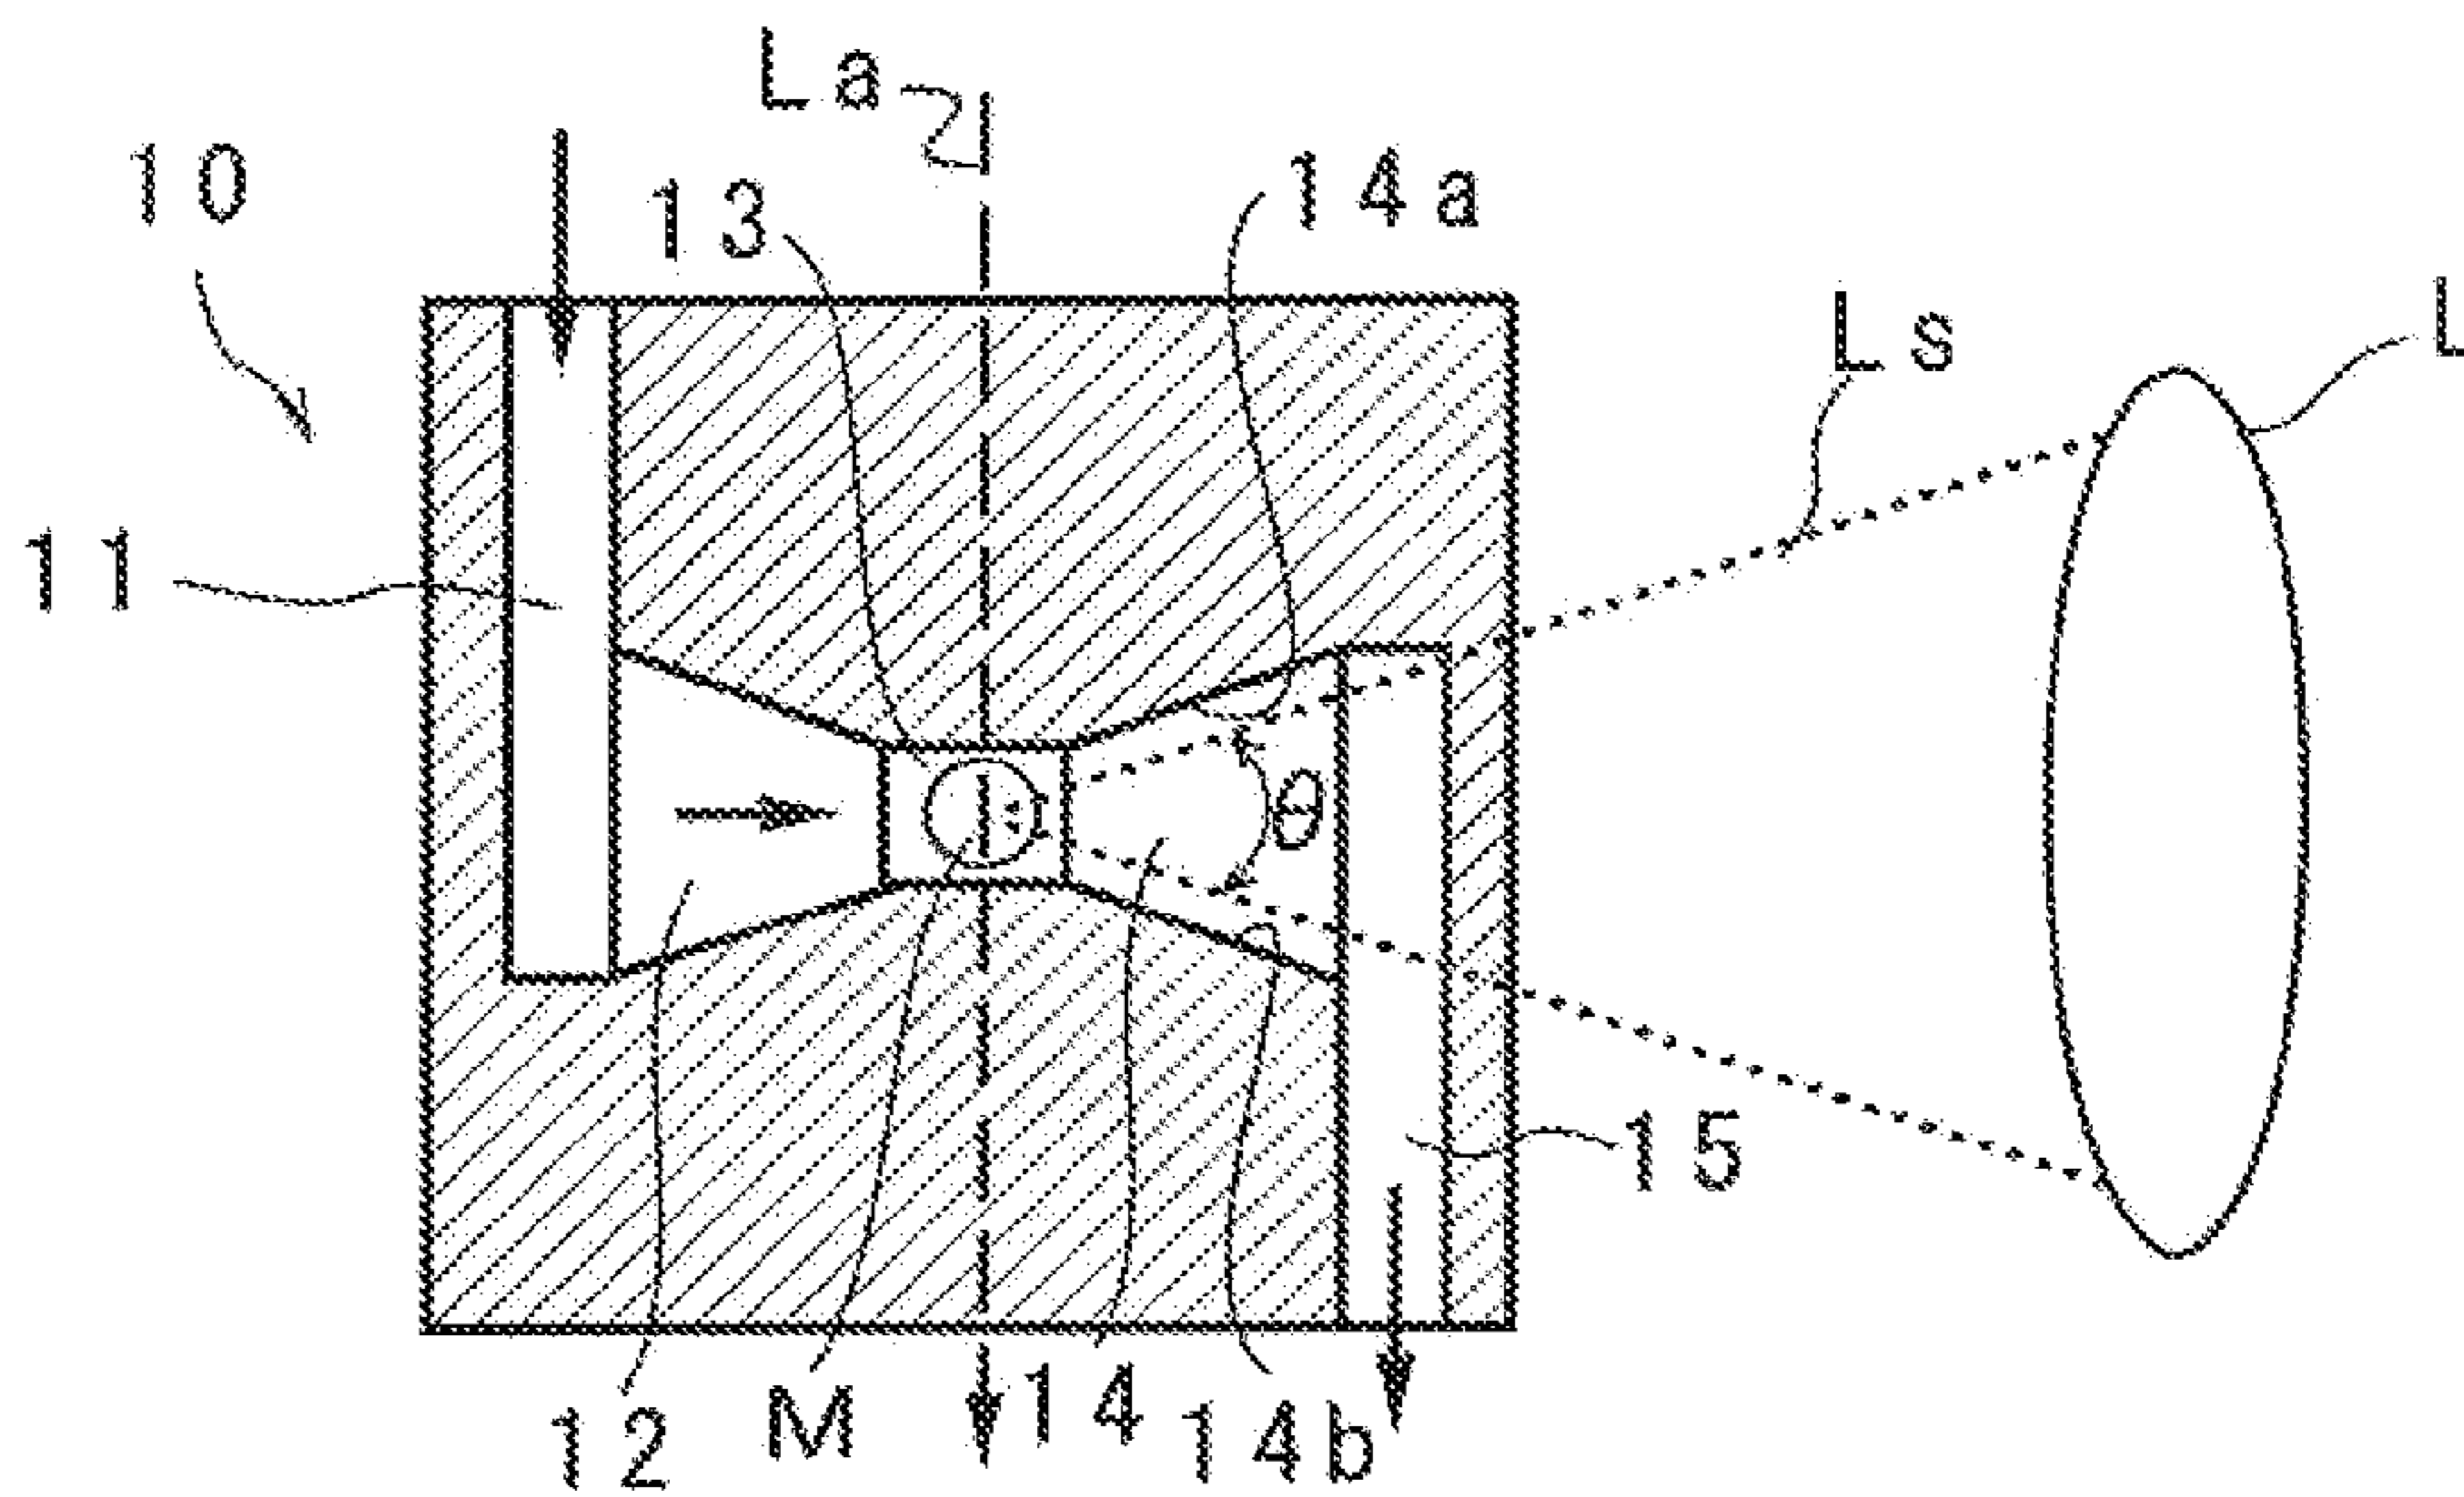


FIG. 4 (b)

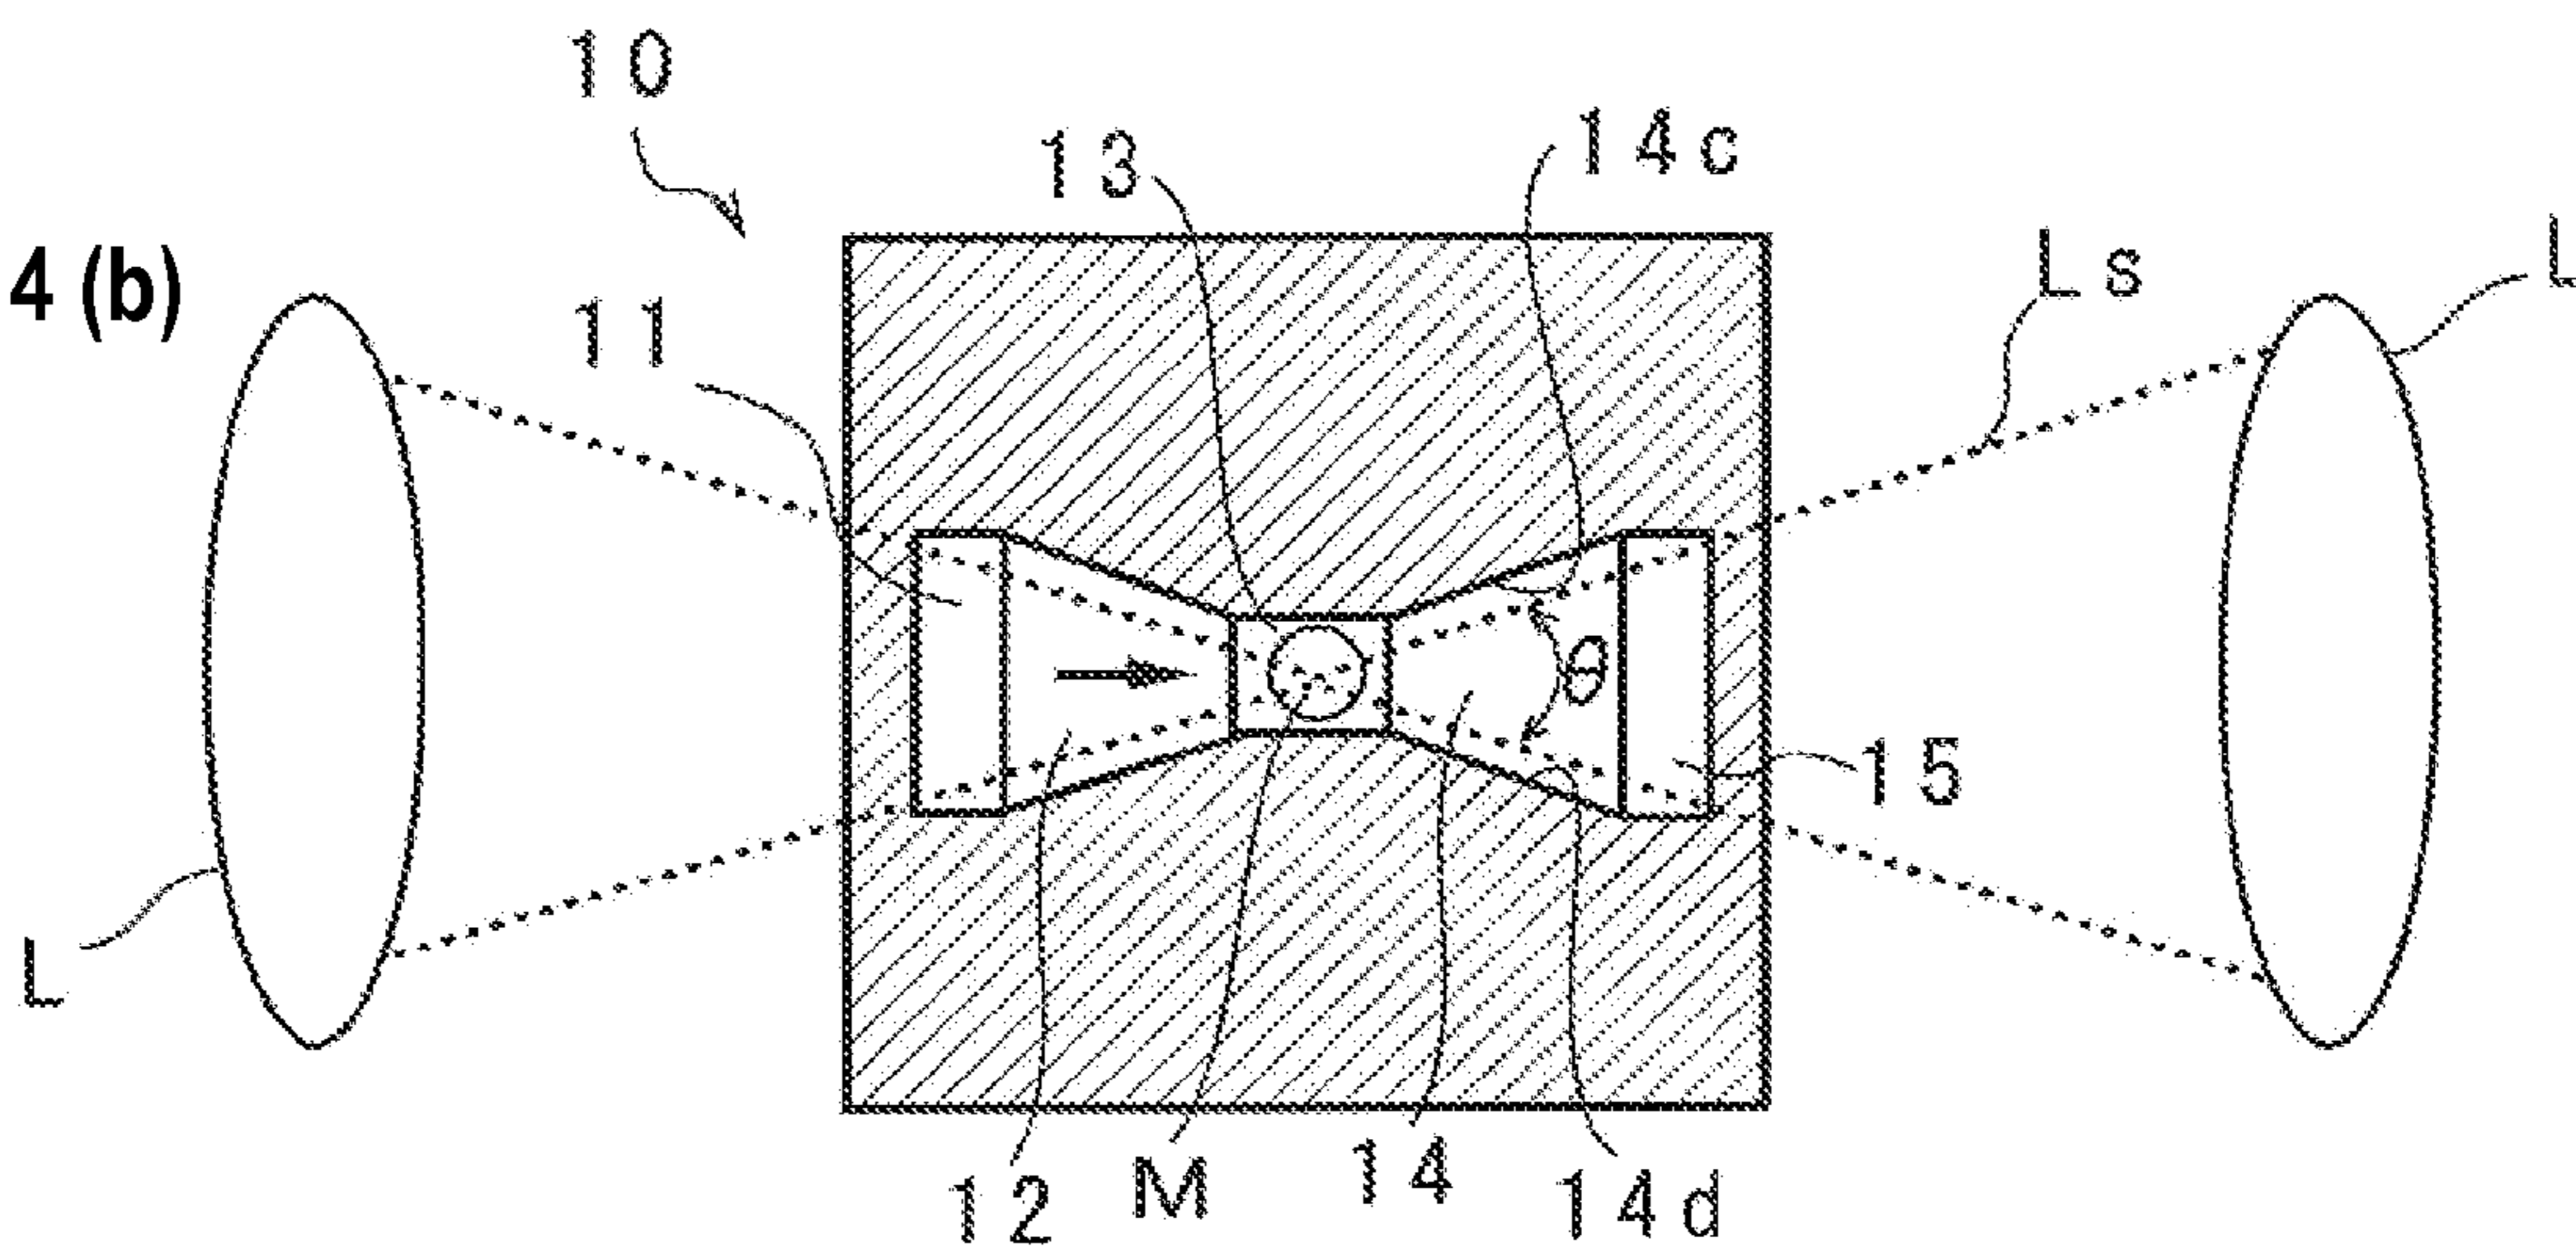


FIG. 5

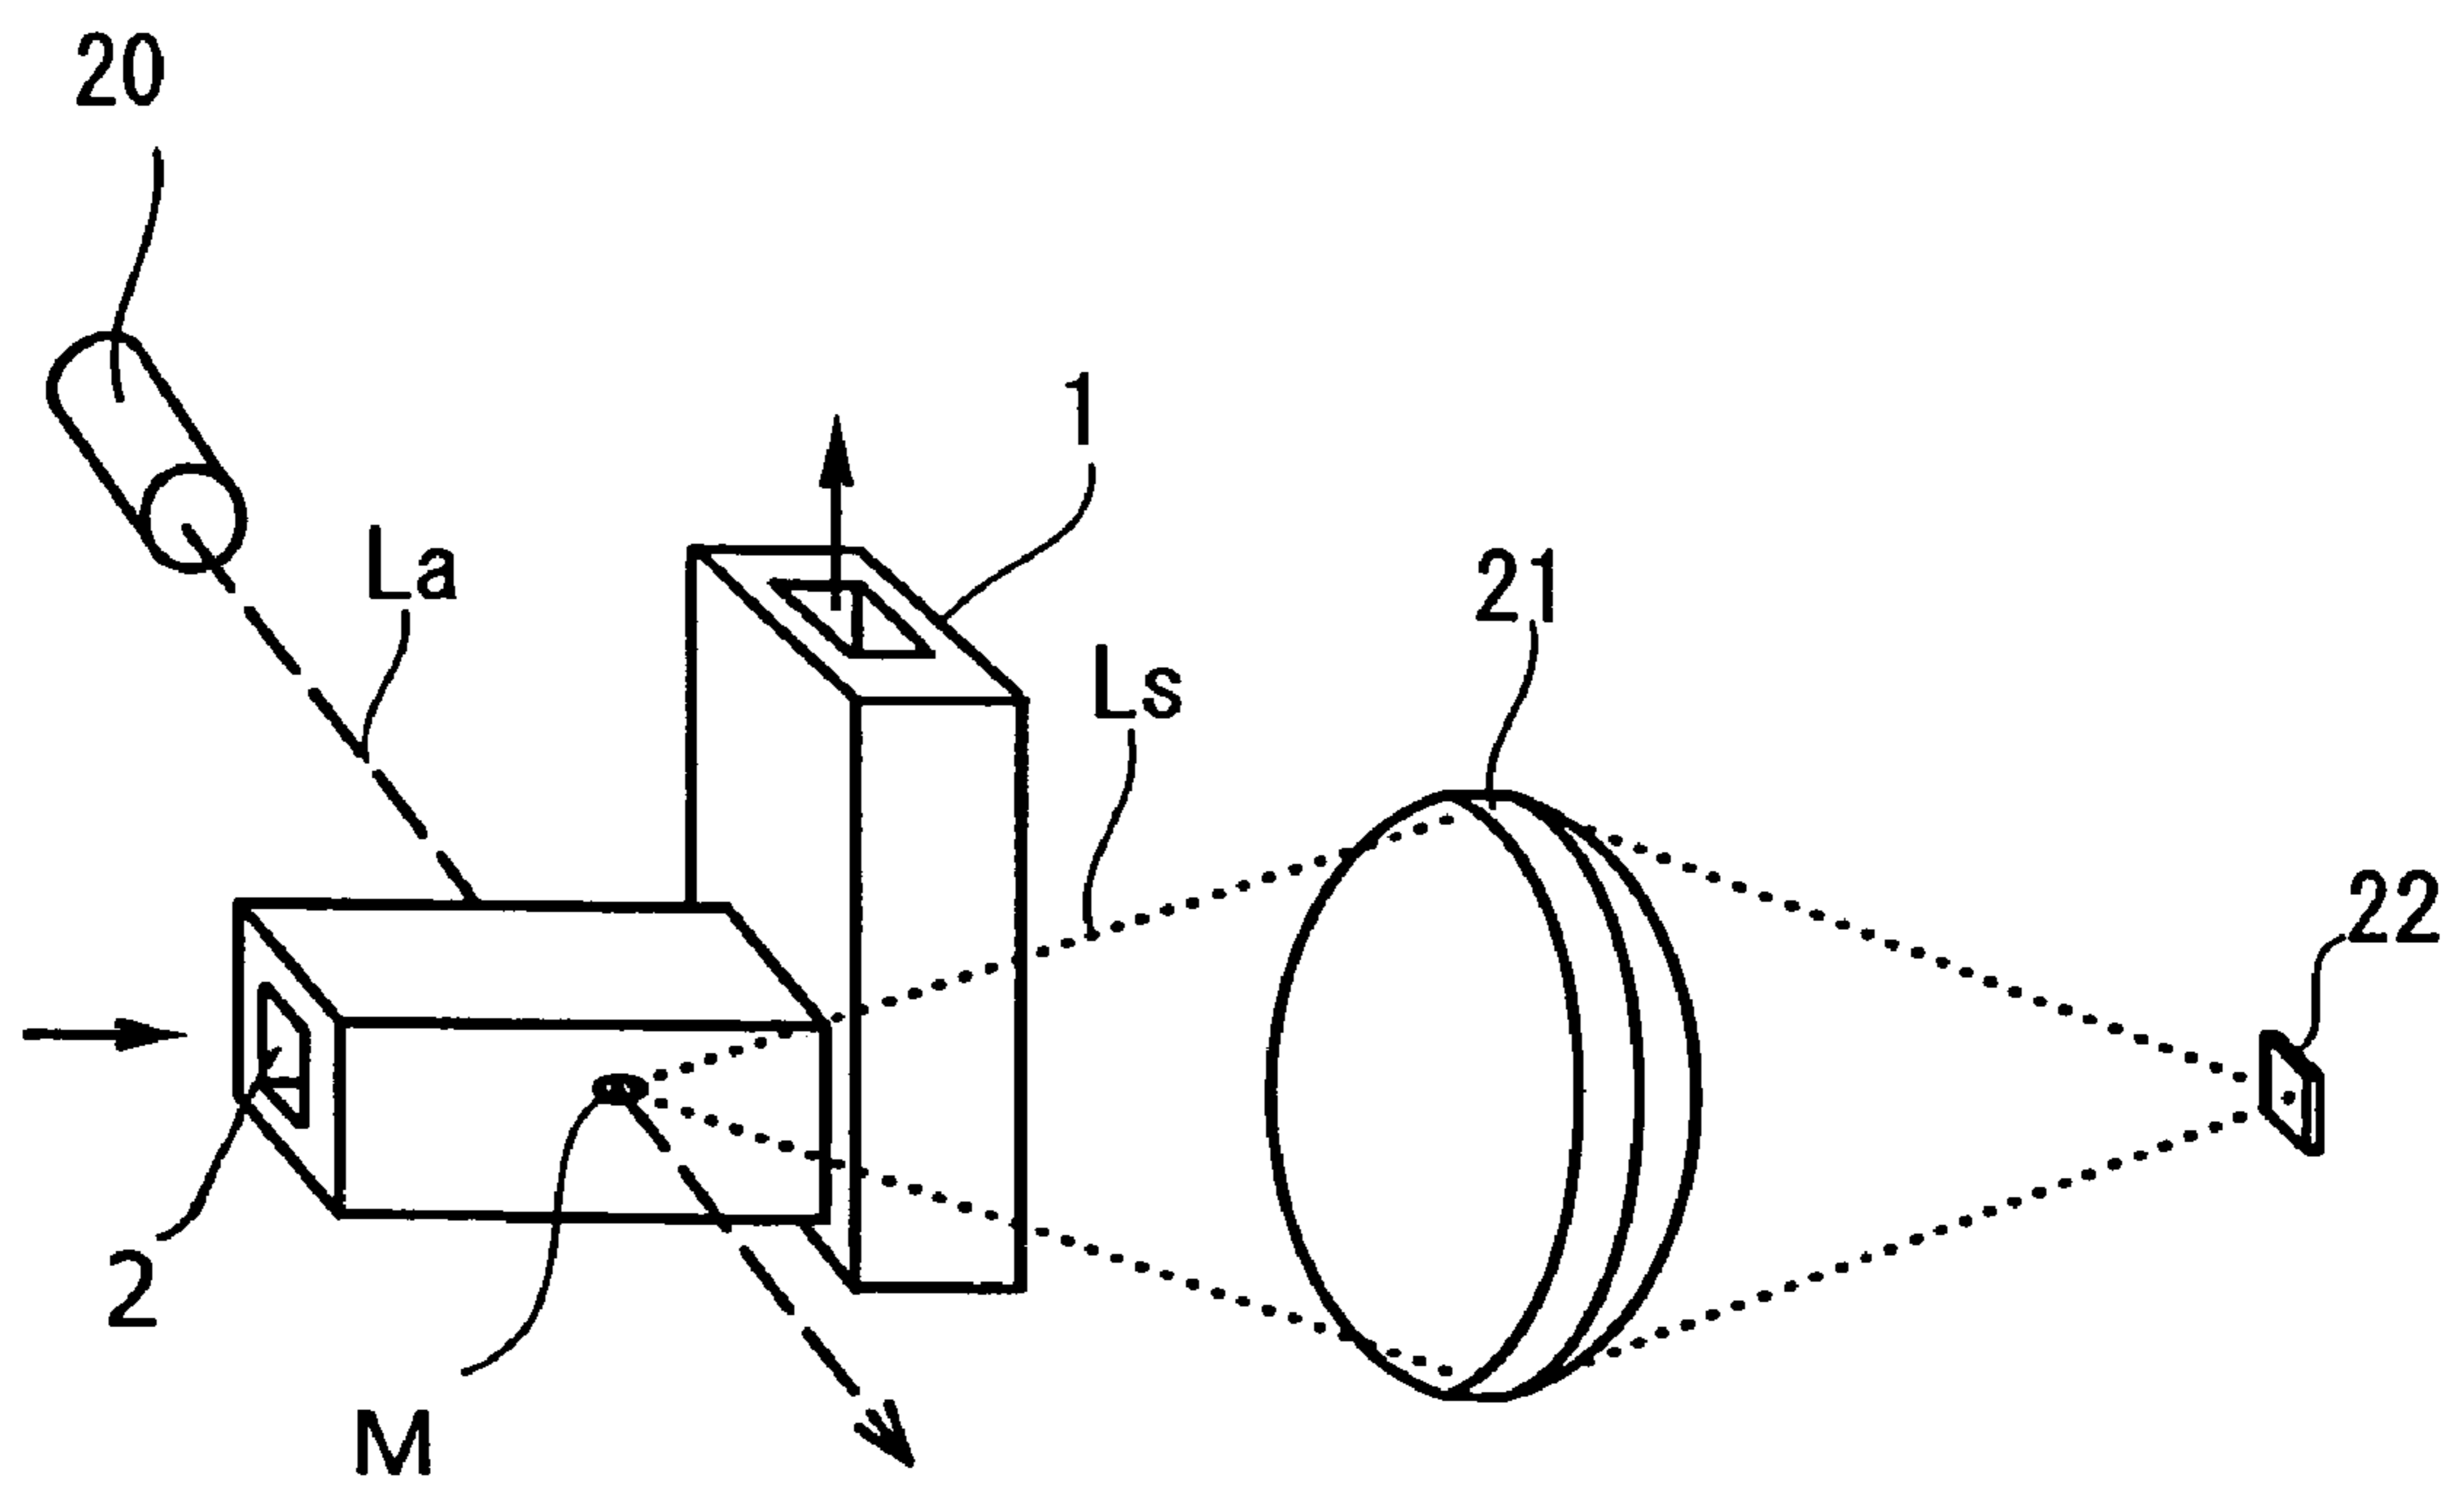


FIG. 6 (a)

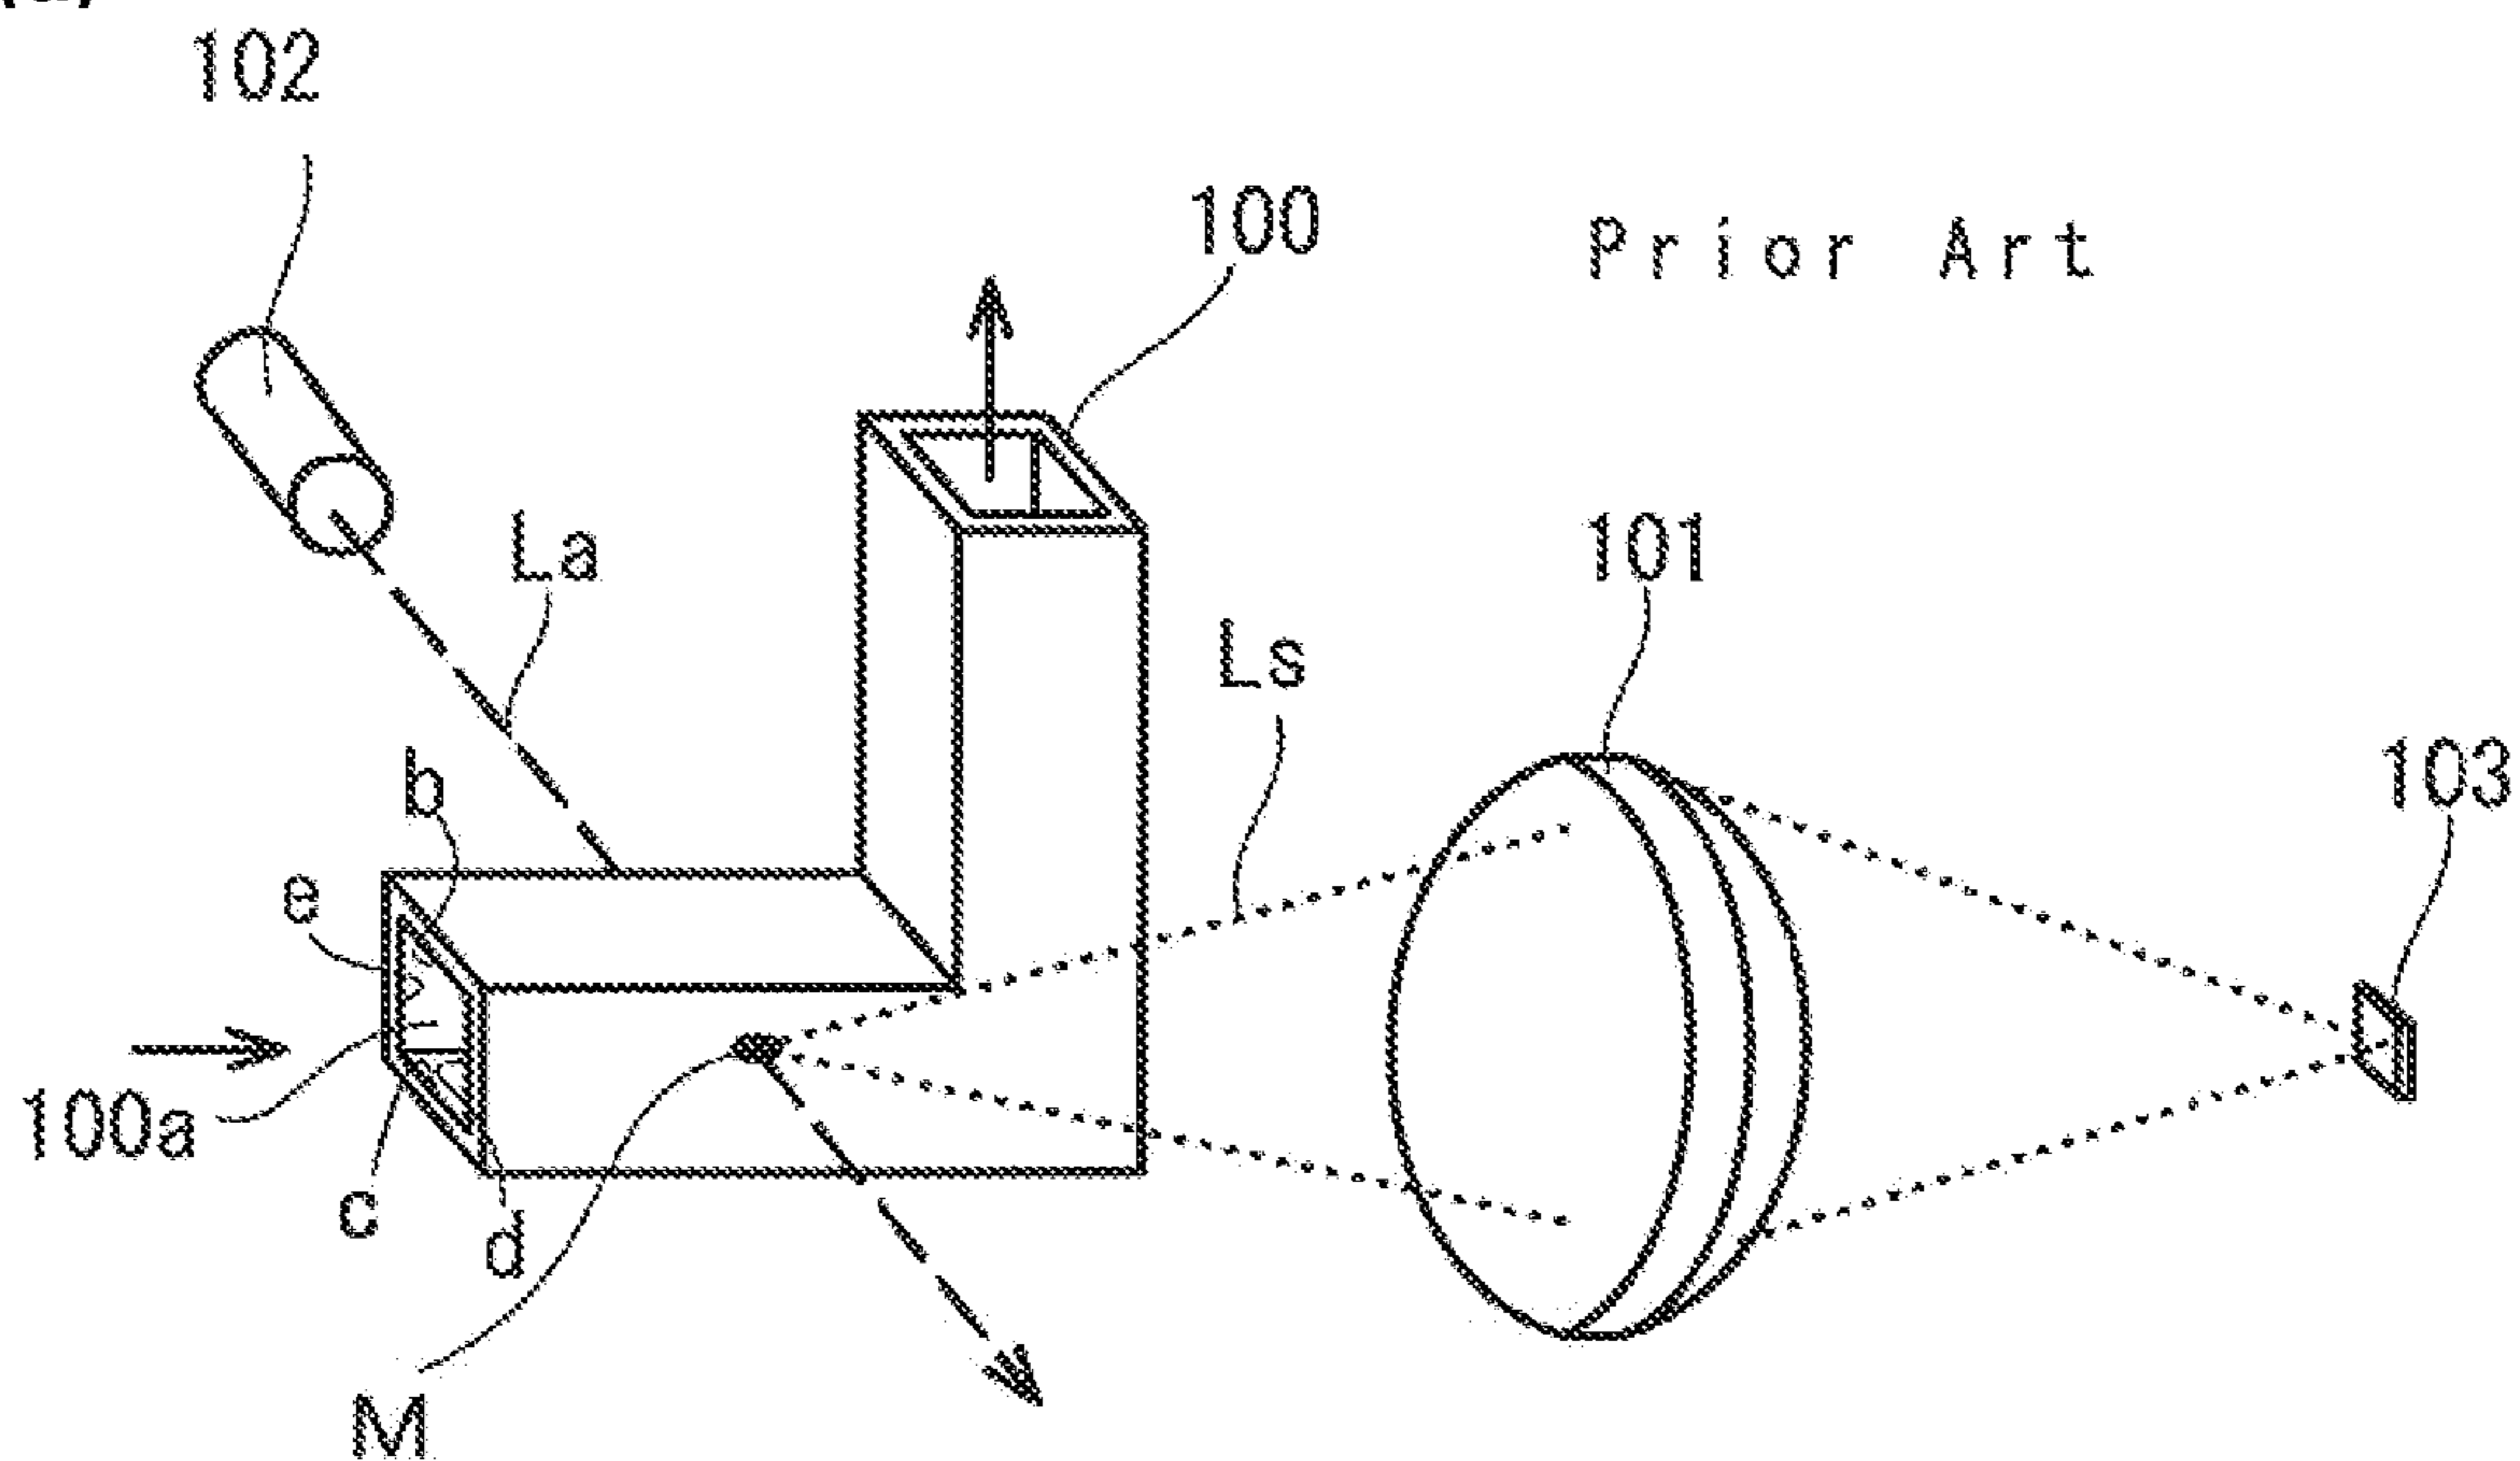


FIG. 6 (b)


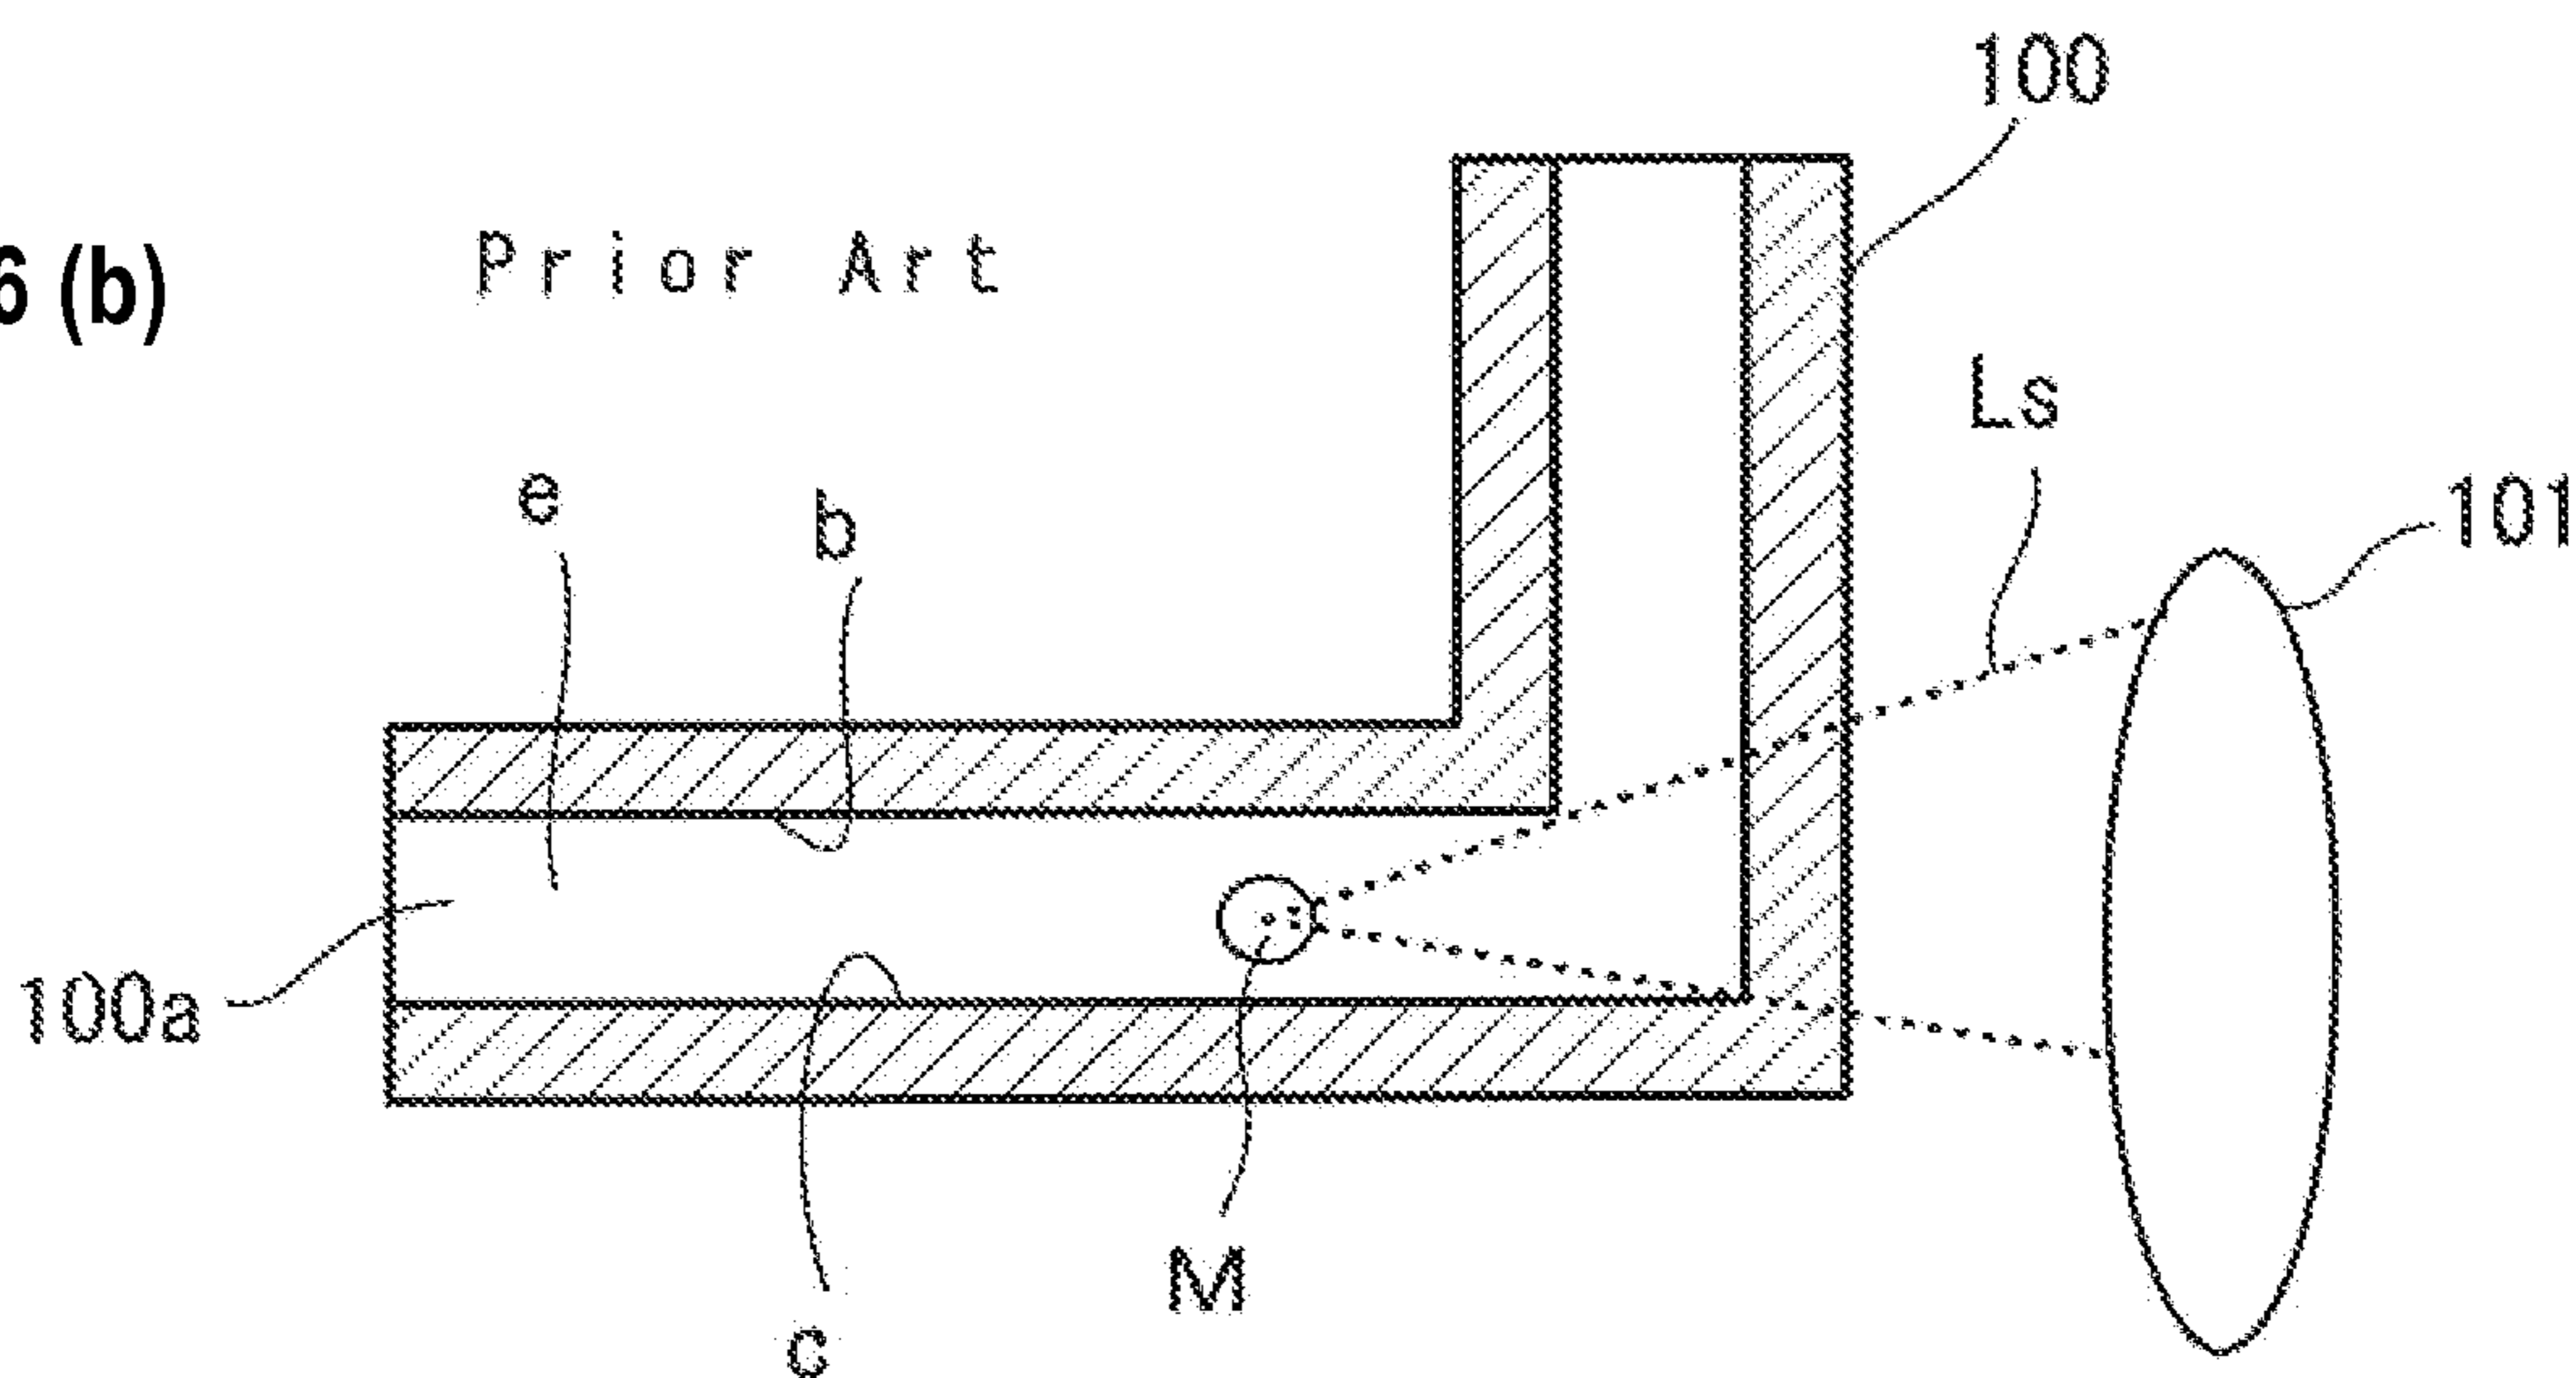


FIG. 6 (c)

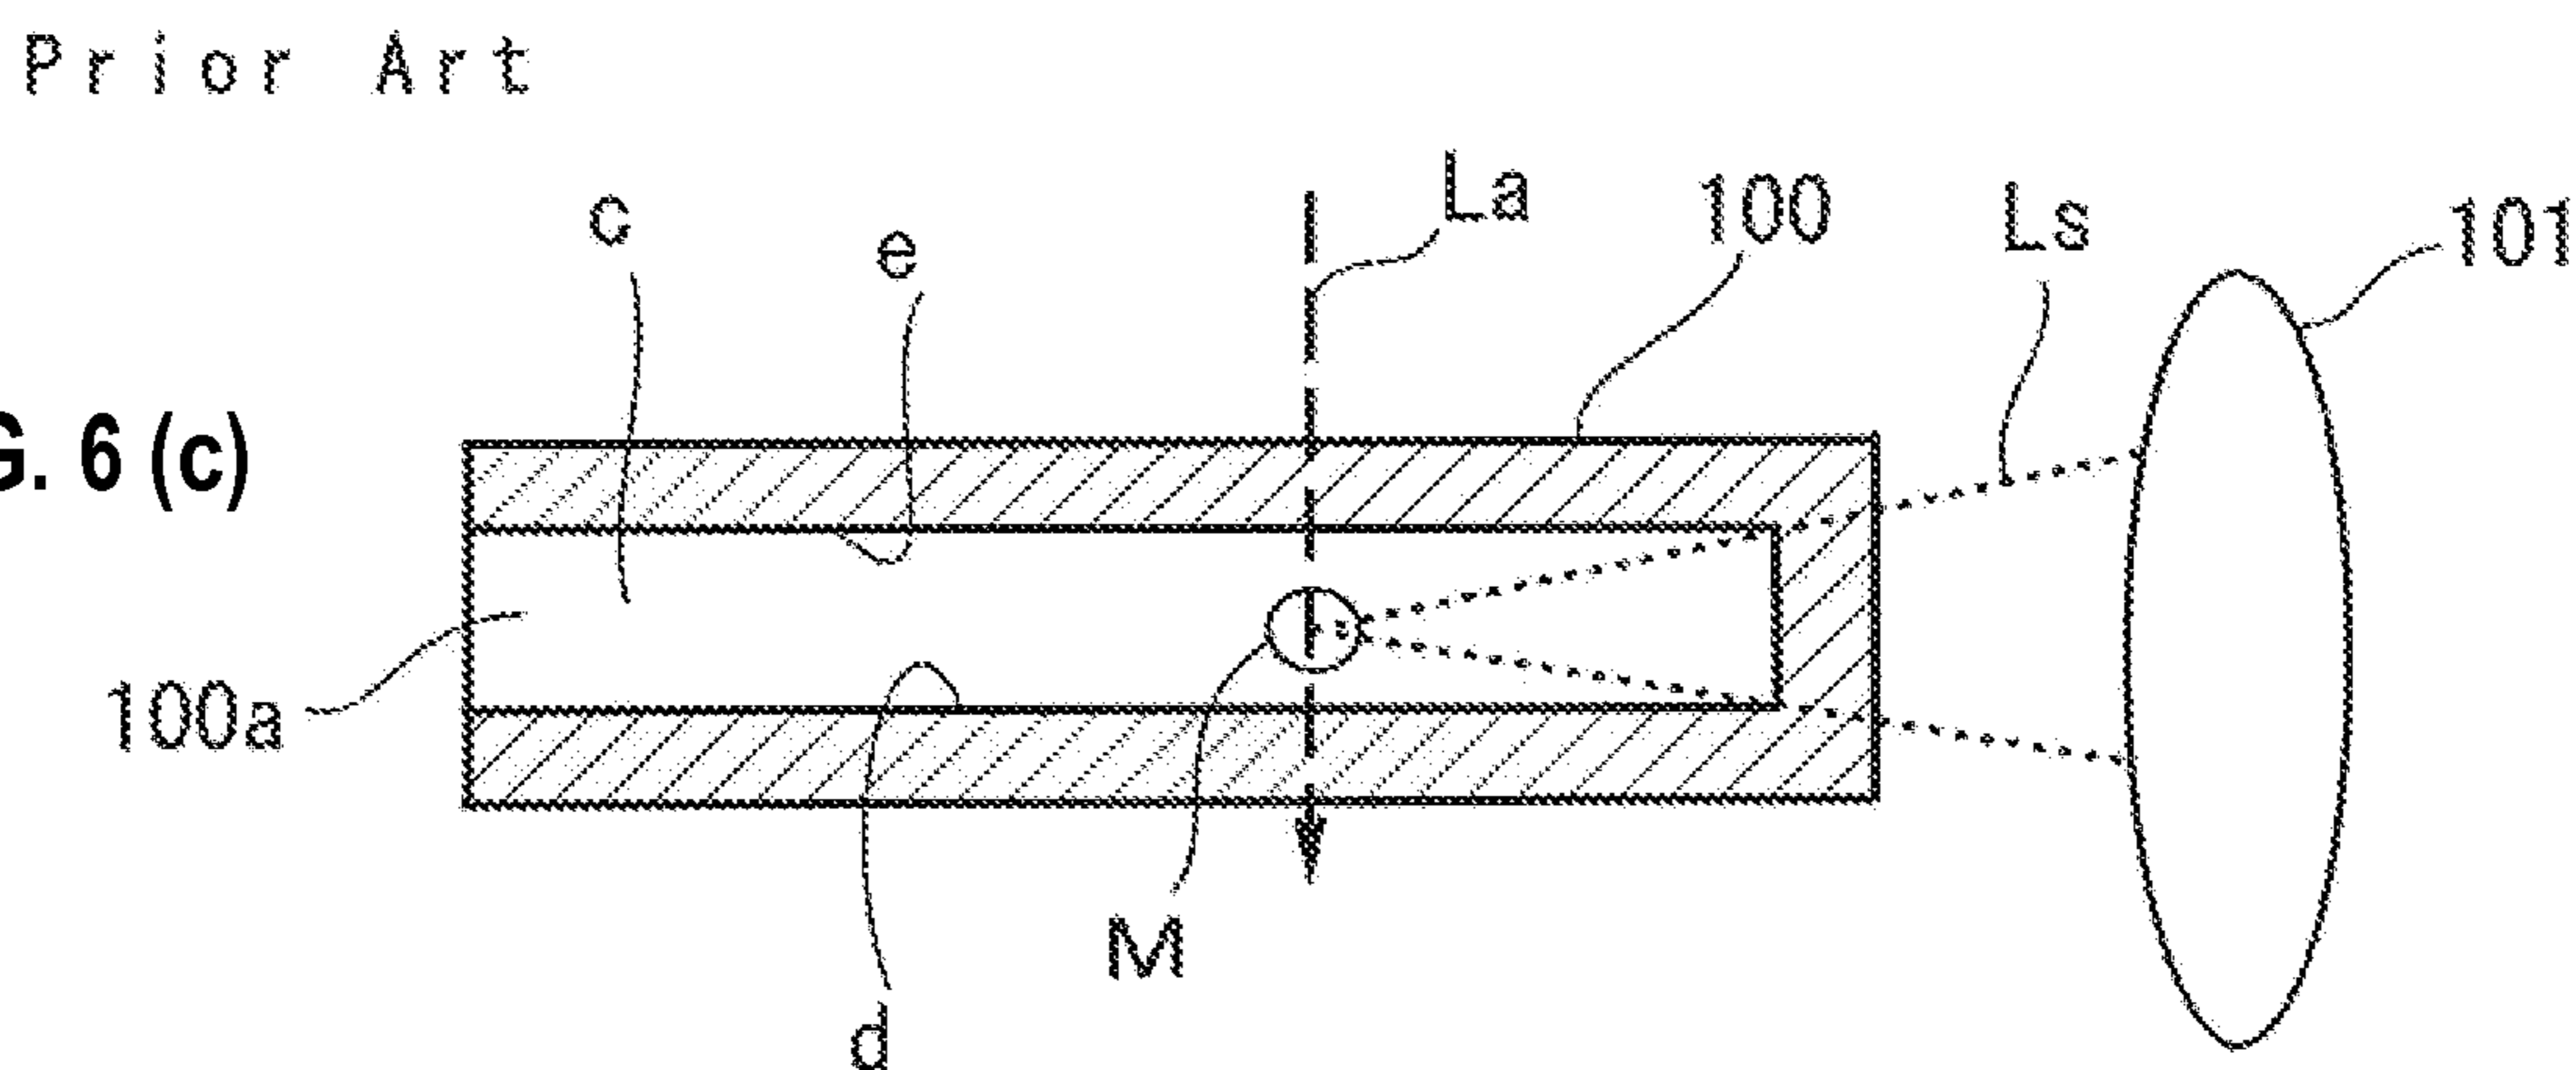

1

**FLOW CELL, AND PARTICLE
MEASUREMENT DEVICE USING THE
SAME**

TECHNICAL FIELD

The present invention relates to a flow cell for flowing sample fluid therethrough to detect light scattered by particles contained in the sample fluid when irradiated with light so as to obtain information such as a particle diameter, and also relates to a particle measuring apparatus using the flow cell.

BACKGROUND ART

A flow cell **100** used for a conventional particle measuring apparatus as shown in FIG. **6(a)** is made of a transparent member, and provided with a linear passage **100a** having a predetermined length, the cross-sectional shape of which is rectangular. Also, the shape of the flow cell is an L-shaped tube as a whole. The central axis of the linear passage **100a** substantially corresponds with the axis of receiving scattered light **Ls** by a condenser lens system **101** (See Japanese Patent Application Publication No. 11-211650). Incidentally, reference number **102** refers to a laser light source, and reference number **103** refers to a photoelectric transducer element.

In the flow cell **100** used for a conventional particle measuring apparatus, inner walls **b**, **c**, **d**, and **e** disadvantageously limit the path of light scattered **Ls** by particles passing through a particle monitoring area **M**, and the condensing angle of the condenser lens system **101** cannot be fully utilized.

Contrary to the conventional apparatus, if the level of detecting scattered light, and hence the accuracy of detecting particles, is to be improved, it is necessary to fully utilize the condensing angle of the condenser lens system **101**.

The present invention was made to solve the above-mentioned drawbacks, and the object of the present invention is to provide a flow cell which can detect scattered light more efficiently by fully utilizing the condensing angle of a condenser means, and also a particle measuring apparatus using the flow cell.

SUMMARY OF THE INVENTION

For solving the above-mentioned drawbacks, according to an aspect of the present invention, there is provided a flow cell in which a particle monitoring area is formed within the flow cell by irradiating the area with light, and light scattered by particles contained in sample fluid passing through the particle monitoring area is condensed by a condenser so as to obtain information including diameter of the particles, wherein inner walls of the flow cell are arranged such that the light scattered by particles is condensed in a state where the condensing angle of the condenser is fully utilized.

According to another aspect of the present invention, there is provided a particle measuring apparatus comprising the above-mentioned flow cell, a light source for irradiating sample fluid flowing through the flow cell to form the particle monitoring area, and an optical detecting and processing means for detecting and processing light scattered or diffracted by particles in the particle monitoring area.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. **1** is a perspective view of the first embodiment of a flow cell according to the present invention;

FIG. **2(a)** is a sectional view seen from direction A—A of FIG. **1** and FIG. **2(b)** is a sectional view seen from direction B—B of FIG. **1**;

2

FIG. **3** is a perspective view of the second embodiment of a flow cell according to the present invention;

FIG. **4(a)** is a sectional view seen from direction C—C of FIG. **3** and FIG. **4(b)**; is a modification thereof including two condenser lenses each placed on opposite sides of the particle measuring apparatus, is a sectional view seen from direction D—D of FIG. **3**;

FIG. **5** shows a schematic structure of a particle measuring apparatus according to the present invention; and

FIG. **6(a)** shows a schematic structure of a conventional particle measuring apparatus, FIG. **6(b)** is a longitudinal sectional view of a conventional flow cell, and FIG. **6(c)** is a cross-sectional view of the conventional flow cell.

DETAILED DESCRIPTION OF THE
INVENTION

Preferred embodiments of the present invention will now be described with reference to the accompanying drawings.

FIG. **1** is a perspective view of the first embodiment of a flow cell according to the present invention, FIG. **2(a)** is a sectional view seen from direction A—A of FIG. **1** and FIG. **2(b)** is a sectional view seen from direction B—B of FIG. **1**, FIG. **3** is a perspective view of the second embodiment of a flow cell according to the present invention, FIG. **4(a)** is a sectional view seen from direction C—C of FIG. **3** and FIG. **4(b)** is a sectional view seen from direction D—D of FIG. **3**, and FIG. **5** shows a schematic structure of a particle measuring apparatus according to the present invention.

As shown in FIGS. **1–2(b)**, the flow cell **1** of the first embodiment is made of a transparent member, and provided with a passage **2** (a first passage) for flowing sample fluid therethrough in a direction of the arrow so as to form a particle monitoring area **M** with respect to laser light **La**, and another passage **3** (a second passage) having two exits at opposite ends which is perpendicular to the passage **2** and located between the passage **2** and a condenser lens **L**. As it will be understood from FIGS. **1–2(b)**, the second passage extends continuously from the first passage; and a width of the second passage is greater than a width of the first passage.

The passage **2** is comprised of four inner walls **2a**, **2b**, **2c**, and **2d**, and the cross section is made rectangular. The passage **3** is also comprised of four inner walls **3a**, **3b**, **3c**, and **3d**, and the cross section is made rectangular.

The particle monitoring area **M** is formed in a position where the four inner walls **2a**, **2b**, **2c**, and **2d** of the passage **2** do not hinder scattered light **Ls** from entering the outmost peripheral portion of the condenser lens **L** for condensing the scattered light **Ls**, so as to fully utilize the condensing angle of the condenser lens **L**.

As shown in FIG. **2(a)**, both ends of the passage **3** are opened. By comparison of FIG. **2(a)** with the conventional flow cell **100** in FIG. **6(b)**, it will be understood that a portion of the inner wall **c** in the linear passage **100a** shown in FIG. **6(b)**, which limits the path of scattered light **Ls**, is effectively removed or eliminated in the flow cell **1**. Consequently, the scattered light **Ls** is not hindered or impeded from entering the outmost periphery portion of the condenser lens **L**.

In addition, as shown in FIG. **2(b)**, the distance between the inner wall **3c** and the inner wall **3d** is arranged to be greater than the distance between the inner wall **2c** and the inner wall **2d** so as not to hinder scattered light **Ls** from entering the outmost peripheral portion of the condenser lens **L** by the inner walls **3c** and **3d**. Conversely, in the conventional flow cell **100** shown in FIGS. **6** and **6(c)**, the distance between walls **d** and **e** is comparable to that between walls

3

b and c such that the walls d and e hinder the scattered light L_s from entering the outmost peripheral portion of the condenser lens L.

In the above-mentioned flow cell **1** of the first embodiment, scattered light L_s generated by particles contained in sample fluid passing through the particle monitoring area M can be condensed in a state where the condensing angle θ of the condenser lens L is fully utilized.

Incidentally, in the first embodiment, both ends of the passage **3** are opened so as to form exits. However, it is also possible to open only one end of the passage **3** and close the other end. In this case, the inner wall for closing the other end must be arranged so as not to hinder scattered light L_s from entering the outmost peripheral portion of the condenser lens L.

Next, as shown in FIGS. **3** and **4**, the flow cell **10** of the second embodiment is made of a transparent member, and provided with a passage **11** having a cross section of a rectangular shape, a passage **12** of a pyramidal shape, a passage **13** having a cross section of a rectangular shape, a passage **14** having a pyramidal shape, and a passage **15** having a cross section of a rectangular shape. The particle monitoring area M is formed within the passage **13** by irradiating sample fluid flowing through the passage **13** in a direction of the arrow with laser light L_a .

The passage **13** is arranged to have a cross-sectional area and a length such that a particle monitoring area M having a desired size can be formed. The passages **11** and **15**, and the passages **12** and **14** are positioned so as to be symmetrical with respect to the center of the passage **13**, respectively.

In addition, as shown in FIGS. **4(a)** and **4(b)**, four inner walls **14a**, **14b**, **14c**, and **14d** of the passage **14** are formed so as not to hinder or impede scattered light L_s from entering the outmost peripheral portion of the condenser lens L. With this, the condensing angle θ of the condenser lens L for condensing the scattered light L_s can be fully utilized.

In the above-mentioned flow cell **10** of the second embodiment, scattered light L_s generated by particles contained in sample fluid passing through the particle monitoring area M can be condensed in a state where the condensing angle θ of the condenser lens L is fully utilized.

Incidentally, in the second embodiment, the passages **12** and **14** are made in a pyramidal shape. However, a conical shape is also possible. Also, another condenser lens L may be provided in the opposite position with respect to the flow cell **10**, on the opposite side of the flow cell from the condensing lens L in FIGS. **4(a)**, **4(b)**, so as to double the scattered light detecting capability. In other words, with two condenser lenses L, L each placed on opposite sides of the flow cell **10**, as shown in FIG. **4(b)**, scattered light detecting capability of the particle measuring apparatus can be doubled.

It is not essential that all portions of the flow cells **1** and **10** are made of a transparent material. It is possible to form the portions where light does not pass with a non-transparent material. In addition, it is not essential that the flow cells **1** and **10** are formed as a unitary member. The same function can be achieved by combing a plurality of members.

Next, as shown in FIG. **5**, the particle measuring apparatus according to the present invention is comprised of the flow cell **1**, a laser light source **20**, a condenser lens system **21** including the condenser lens L, and a photoelectric transducer element **22**. The flow cell **10** shown in FIG. **3** can be used instead of the flow cell **1** in such apparatus.

The particle monitoring area M is formed by irradiating a predetermined area of the passage **2** of the flow cell **1** with laser light L_a from the laser light source **20**. The optical axis

4

of the laser light L_s is substantially perpendicular to the central axis of the passage **2** within the flow cell **1**.

The condenser lens system **21** has an optical axis which corresponds to the central axis of the passage **2**, and condenses scattered light L_s generated by particles which has been irradiated with the laser light L_a in the particle monitoring area M. Incidentally, the condenser lens system **21** does not always need to be positioned on the central axis of the passage **2**.

The photoelectric transducer element **22** is provided on the optical axis of the condenser lens system **21**, and receives the scattered light L_s which has been condensed by the condenser lens system **21** so as to transduce the scattered light L_s into voltage, which varies depending on the intensity of the scattered light L_s . The condenser lens system **21** and subsequent elements are referred to as an optical detecting and processing means.

In operation, a predetermined area of the passage **2** is irradiated with laser light L_a which has been emitted from the laser light source **20** so as to form a particle monitoring area M. When particles contained in sample fluid pass through the particle monitoring area M, the particles are irradiated with the laser light L_a and scattered light L_s is generated.

The scattered light L_s is condensed by the condenser lens system **21** toward the photoelectric transducer element **22** in a state where the condensing angle of the condenser lens system **21** is fully utilized due to the shape of the passages **2** and **3**. Next, the scattered light L_s which has been condensed toward the photoelectric transducer element **22** is transduced into voltage which varies depending on the intensity of the scattered light L_s .

Since the shape of the passages **2** and **3** is arranged such that the condenser lens system **21** can condense the scattered light L_s toward the photoelectric transducer element **22** in a state where the condensing angle θ is fully utilized, the detection level can be improved.

INDUSTRIAL APPLICABILITY

As mentioned above, according to an aspect of the present invention, scattered light generated by particles contained in sample fluid passing through the particle monitoring area can be condensed in a state where the condensing angle of the condenser means is fully utilized.

According to another aspect of the present invention, since the shape of the passage of the flow cell is arranged such that optical detecting and processing means can condense the scattered light in a state where the condensing angle is fully utilized, the detection level can be improved.

Although there have been disclosed what are the present embodiments of the invention, it will be understood that variations and modifications may be made thereto without departing from the spirit of scope of the invention as indicated by the appended claims.

The invention claimed is:

1. A particle measuring apparatus comprising:
 - a flow cell having a first passage and a second passage extending continuously from the first passage;
 - a particle monitoring area formed in the first passage by irradiating the flow cell with light; and
 - a condenser which condenses light scattered by particles contained in sample fluid passing through the particle monitoring area so as to obtain information including diameter of the particles,
 wherein a central axis of the first passage substantially corresponds to an optical axis of the condenser, and

5

a width of the second passage is greater than a width of the first passage so as not to impede the scattered light from entering an outmost peripheral portion of the condenser.

2. The particle measuring apparatus according to claim 1, wherein the second passage is substantially perpendicular to the first passage.

3. The particle measuring apparatus according to claim 2, wherein inner walls of the flow cell define an opening communicating said first and second passages, and said opening being sufficiently large so as not to impede the scattered light from entering the outmost peripheral portion of the condenser.

4. The particle measuring apparatus according to claim 2, wherein the second passage has a substantially rectangular cross sectional shape.

5. The particle measuring apparatus according to claim 1, wherein the second passage includes one of a pyramidal shape and a conical shape, and a central axis of the second passage substantially corresponds to that of the first passage.

6. The particle measuring apparatus according to claim 5, wherein the condenser has a condensing angle which is substantially fully utilized for condensing the light scattered by the particles.

7. The particle measuring apparatus according to claim 1, wherein the flow cell further comprises:

second passages having one of a pyramidal shape and a conical shape provided on an upstream side and a downstream side of the flow cell, respectively; and another condenser;

wherein

central axes of the second passages substantially correspond to that of the first passage, and said condensers are provided on opposite sides of the flow cell.

8. The particle measuring apparatus according to claim 7, wherein the condenser has a condensing angle which is substantially fully utilized for condensing the light scattered by the particles.

9. The particle measuring apparatus according to claim 7, wherein the condensers are condensing lenses.

10. The particle measuring apparatus according to claim 1, wherein the condenser is a condensing lens.

11. The particle measuring apparatus according to claim 1, wherein the first passage has a substantially rectangular cross sectional shape.

12. A particle measuring apparatus comprising:

a flow cell having a first passage and a second passage extending continuously from the first passage;

a particle monitoring area formed in the first passage by irradiating the flow cell with light; and

a condenser which condenses light scattered by particles contained in sample fluid passing through the particle monitoring area so as to obtain information including diameter of the particles; wherein

a central axis of the first passage substantially corresponds to an optical axis of the condenser; and

a width of the second passage is greater than a width of the first passage so as not to impede the scattered light

6

from entering an outmost peripheral portion of the condenser at a position where the condenser is arranged relative to the flow cell.

13. The particle measuring apparatus according to claim 12, wherein the second passage which is substantially perpendicular to the first passage and extends continuously therefrom.

14. The particle measuring apparatus according to claim 12, wherein the second passage includes one of a pyramidal shape and a conical shape and extending continuously from the first passage, and a central axis of the second passage substantially corresponds to that of the first passage.

15. The particle measuring apparatus according to claim 12, wherein the flow cell further comprises:

second passages having a pyramidal shape or a conical shape provided on an upstream side and a downstream side of the flow cell, respectively, and which extend continuously from the first passage; and

another condenser; wherein

central axes of the sub passages substantially correspond to that of the first passage, and said condensers are provided on opposite sides of the flow cell.

16. A particle measuring apparatus comprising:

a flow cell having a first passage and second passage extending continuously from the said first passage;

a particle monitoring area formed in the first passage by irradiating the flow cell with light; and

a plurality of condensers which condense light scattered by particles contained in sample fluid passing through the particle monitoring area so as to obtain information including diameter of the particles,

wherein

a central axis of the first passage substantially corresponds to an optical axis of the condensers and inner walls of the flow cell are arranged so as not to impede the scattered light from entering outmost peripheral portions of the condensers;

said condensers are provided on opposite sides of the flow cell; and

a width of the second passages is greater than a width of the first passage so as not to impede the scattered light from entering the outmost peripheral portions of the condensers.

17. The particle measuring apparatus according to claim 16, wherein the condensers are condensing lenses.

18. The particle measuring apparatus according to claim 16, wherein the second passages are disposed substantially perpendicular to the first passage.

19. The particle measuring apparatus according to claim 18, wherein the second passage extends continuously from the first passage.

20. The particle measuring apparatus according to claim 18, wherein a width of the second is greater than a width of the first passage.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 7,170,601 B2
APPLICATION NO. : 10/528900
DATED : January 30, 2007
INVENTOR(S) : Matsuda

Page 1 of 2

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page:

In the title, section (54), change “**FLOW CELL, AND PARTICLE MEASUREMENT DEVICE USING THE SAME**” to **--FLOW CELL AND PARTICLE MEASURING APPARATUS USING THE SAME--**.

After the abstract, section (57), change “**20 Claims, 4 Drawing Sheets**” to **--18 Claims, 4 Drawing Sheets--**.

Column 1:

Line 1, change “**FLOW CELL, AND PARTICLE**” to **--FLOW CELL AND PARTICLE--**.

Line 2, change “**MEASUREMENT DEVICE USING THE**” to **--MEASURING APPARATUS USING THE--**.

Column 2:

Line 4, change “**FIG. 3 and FIG. 4(b); is a modification**” to **--FIG. 3, and FIG. 4(b) is a modification--**.

Line 59, change “**the outmost periphery portion**” to **--the outmost peripheral portion--**.

Column 3:

Line 58, change “**achieved by combing a plurality**” to **--achieved by combining a plurality--**.

Column 4:

Line 54, change “**spirit of scope**” to **--spirit or scope--**.

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 7,170,601 B2
APPLICATION NO. : 10/528900
DATED : January 30, 2007
INVENTOR(S) : Matsuda

Page 2 of 2

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Column 6:

Line 20, change "axes of the sub passages" to --axes of the second passages--.


Line 25, change "first passage and second passage" to --first passage and second passages--.

Line 26, change "from the said" to --from said--.

Lines 51-56, delete Claims 19 and 20.

Signed and Sealed this

Eighteenth Day of March, 2008

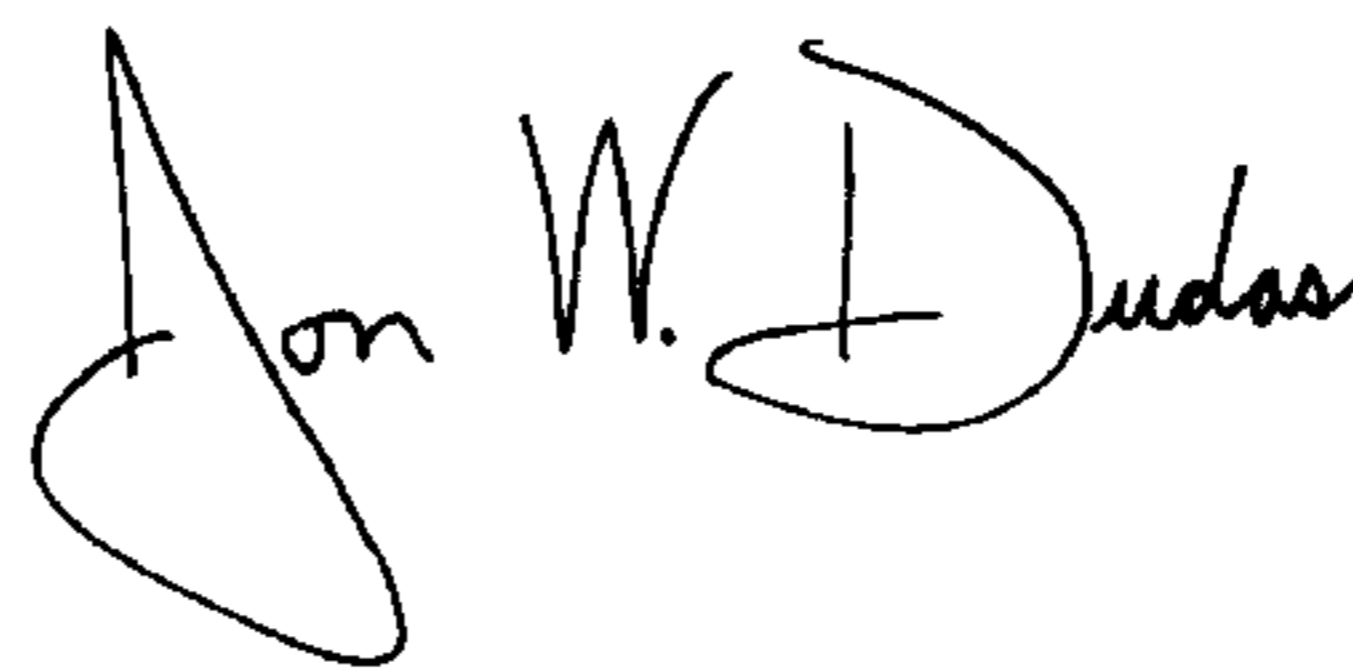A handwritten signature in black ink that reads "Jon W. Dudas". The signature is written in a cursive style with a large, stylized initial "J" and "D".

JON W. DUDAS

Director of the United States Patent and Trademark Office