

US007642451B2

(12) **United States Patent**
Bonn

(10) **Patent No.:** **US 7,642,451 B2**
(45) **Date of Patent:** **Jan. 5, 2010**

(54) **THERMALLY TUNED COAXIAL CABLE FOR MICROWAVE ANTENNAS**

(75) Inventor: **Kenlyn S. Bonn**, Boulder, CO (US)

(73) Assignee: **Vivant Medical, Inc.**, Boulder, CO (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **12/351,633**

(22) Filed: **Jan. 9, 2009**

(65) **Prior Publication Data**

US 2009/0183895 A1 Jul. 23, 2009

Related U.S. Application Data

(60) Provisional application No. 61/023,029, filed on Jan. 23, 2008.

(51) **Int. Cl.**
H01B 11/00 (2006.01)

(52) **U.S. Cl.** **174/28**; 174/102 R; 174/102 SP;
174/102 P

(58) **Field of Classification Search** 174/36,
174/102 R, 102 SP, 102 P, 28, 29, 117 AS,
174/113 AS, 115, 116, 121 R; 333/84 L,
333/237

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,599,857 A * 6/1952 Mildner 264/145
3,761,332 A * 9/1973 Jachimowicz et al 156/55
4,011,118 A * 3/1977 Geominy 156/51
4,018,977 A * 4/1977 Herrmann et al. 174/24

5,262,593 A * 11/1993 Madry et al. 174/102 R
5,344,441 A 9/1994 Gronauer
5,369,251 A 11/1994 King et al.
5,810,803 A 9/1998 Moss et al.
6,026,331 A 2/2000 Feldberg et al.
6,287,302 B1 9/2001 Berube
6,346,671 B1 * 2/2002 Ahrens et al. 174/28
6,527,768 B2 3/2003 Berube
6,878,147 B2 4/2005 Prakash et al.
7,147,632 B2 12/2006 Prakash et al.
7,194,297 B2 3/2007 Talpade et al.
7,244,254 B2 7/2007 Brace et al.

FOREIGN PATENT DOCUMENTS

DE 390937 3/1924
DE 1099658 2/1961
DE 1139927 11/1962
DE 1149832 6/1963

(Continued)

OTHER PUBLICATIONS

U.S. Appl. No. 08/483,742, filed Jun. 7, 1995.


(Continued)

Primary Examiner—William H Mayo, III

(57) **ABSTRACT**

A coaxial cable, including an outer conductor and an inner conductor adapted to connect to an energy source for treating tissue and first and second dielectric materials disposed between the inner conductor and the outer conductor which position the inner conductor relative to the outer conductor in general concentric relation thereto. The first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion.

20 Claims, 8 Drawing Sheets

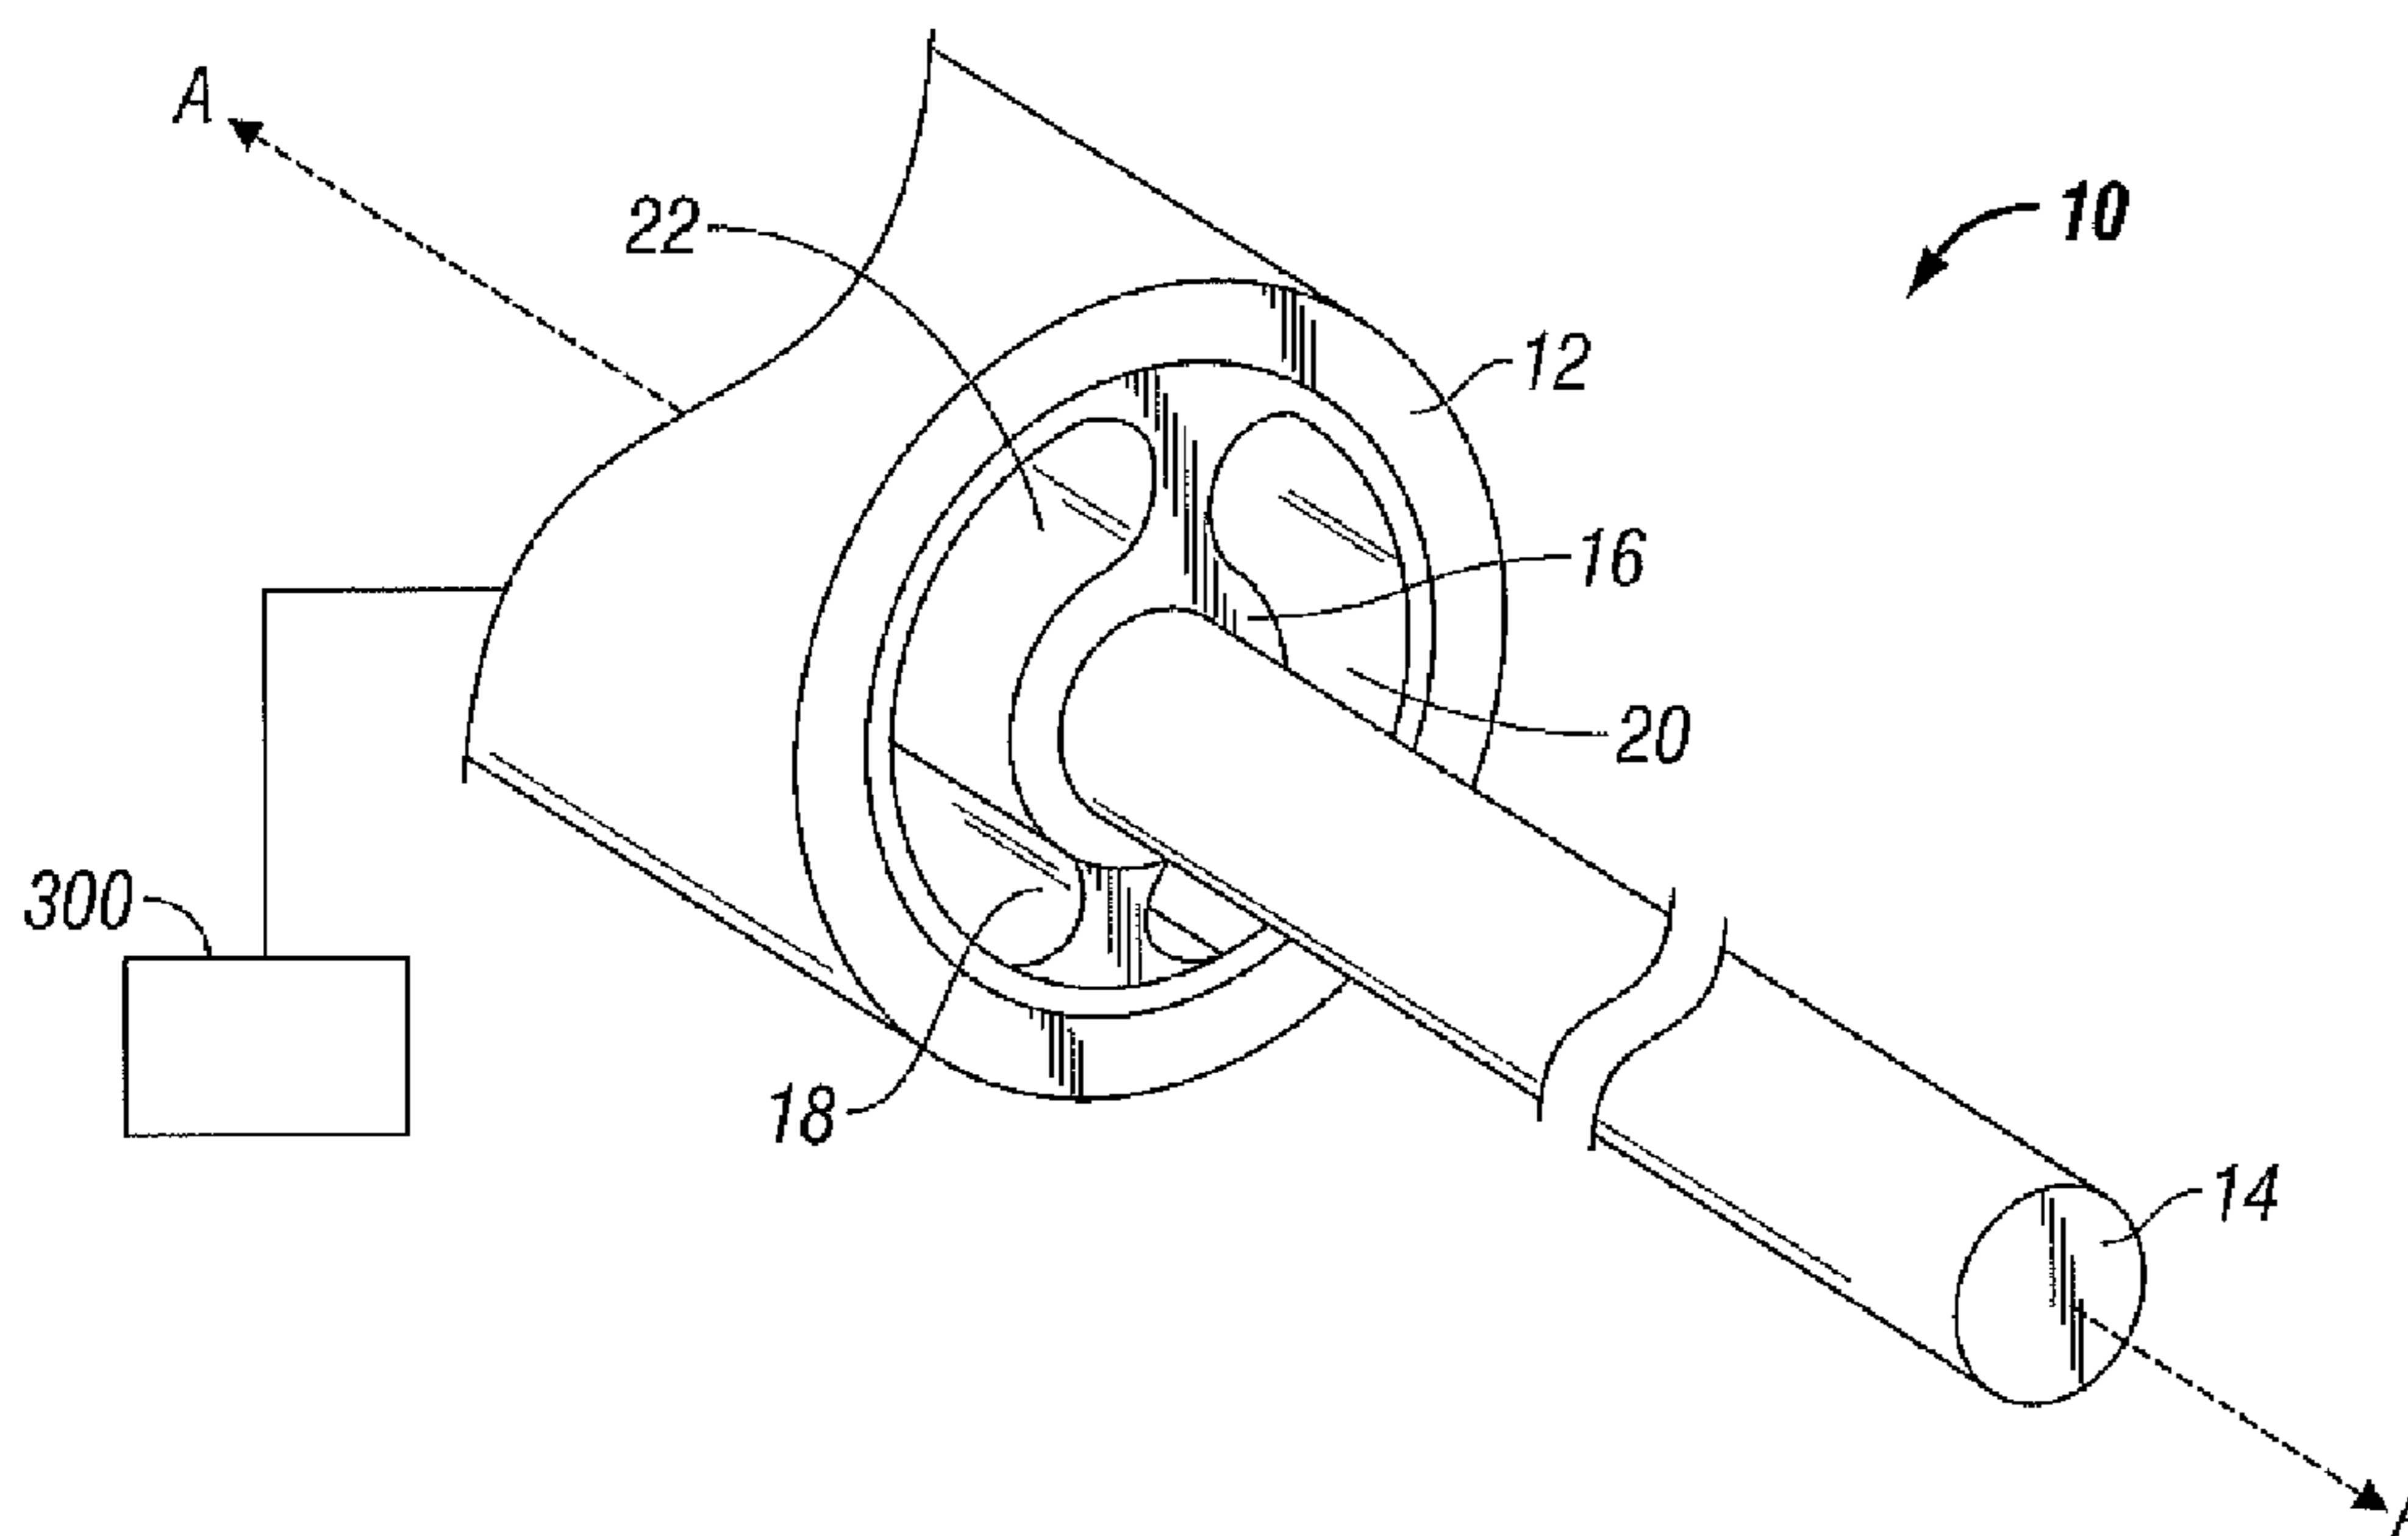

FOREIGN PATENT DOCUMENTS		
DE	1439302	1/1969
DE	2439587	2/1975
DE	2455174	5/1975
DE	2407559	8/1975
DE	2415263	10/1975
DE	2429021	1/1976
DE	2460481	6/1976
DE	2602517	7/1976
DE	2504280	8/1976
DE	2627679	1/1977
DE	2540968	3/1977
DE	2820908	11/1978
DE	2803275	8/1979
DE	2823291	11/1979
DE	2946728	5/1981
DE	3143421	5/1982
DE	3045996	7/1982
DE	3120102	12/1982
DE	3510586	10/1986
DE	3604823	8/1987
DE	8712328	3/1988
DE	3711511	6/1988
DE	3904558	8/1990
DE	3942998	7/1991
DE	4238263	5/1993
DE	4303882	8/1994
DE	4339049	5/1995
DE	29616210	1/1997
DE	19608716	4/1997
DE	19751106	5/1998
DE	19717411	11/1998
DE	19751108	5/1999
DE	19801173	7/1999
DE	19848540	5/2000
DE	10224154	12/2003
DE	10328514	3/2005
DE	102004022206	12/2005
DE	202005015147	3/2006
EP	0 246 350	11/1987
EP	0 481 685	4/1992
EP	0 521 264	1/1993
EP	0 541 930	5/1993
EP	0 556 705	8/1993
EP	0 558 429	9/1993
EP	0 572 131	12/1993
EP	0 836 868	4/1998
EP	1 159 926	5/2001
FR	179607	11/1906
FR	1 275 415	9/1960
FR	1 347 865	11/1963
FR	2 276 027	6/1974
FR	2 235 669	1/1975
FR	2 313 708	12/1976
FR	2 502 935	10/1982
FR	2 517 953	6/1983
FR	2 573 301	11/1984
FR	2 862 813	5/2005
FR	2 864 439	7/2005
JP	5-5106	1/1993
JP	05-40112	2/1993
JP	06343644	12/1994
JP	07265328	10/1995
JP	08056955	3/1996
JP	08252263	10/1996
JP	09010223	1/1997
JP	11244298	9/1999
JP	2000342599	12/2000
JP	2000350732	12/2000
JP	2001008944	1/2001
JP	2001029356	2/2001
JP	2001128990	5/2001

SU	166452	11/1964
SU	401367	11/1974
SU	727201	4/1980

OTHER PUBLICATIONS

U.S. Appl. No. 08/136,098, filed Oct. 14, 1993.
U.S. Appl. No. 09/195,118, filed Nov. 18, 1998.
U.S. Appl. No. 10/244,346, filed Sep. 16, 2002.
U.S. Appl. No. 11/053,987, filed Feb. 08, 2005.
U.S. Appl. No. 12/023,606, filed Jan. 31, 2008.
U.S. Appl. No. 12/129,482, filed May 29, 2008.
U.S. Appl. No. 12/135,425, filed Jun. 09, 2008.
U.S. Appl. No. 12/135,690, filed Jun. 09, 2008.
U.S. Appl. No. 12/147,093, filed Jun. 26, 2008.
U.S. Appl. No. 12/181,504, filed Jul. 29, 2008.
U.S. Appl. No. 12/184,556, filed Aug. 01, 2008.
U.S. Appl. No. 12/194,254, filed Aug. 19, 2008.
U.S. Appl. No. 12/197,601, filed Aug. 25, 2008.
U.S. Appl. No. 12/197,405, filed Aug. 25, 2008.
U.S. Appl. No. 12/197,473, filed Aug. 25, 2008.
U.S. Appl. No. 12/199,935, filed Aug. 28, 2008.
U.S. Appl. No. 12/203,474, filed Sep. 3, 2008.
U.S. Appl. No. 12/236,686, filed Sep. 24, 2008.
U.S. Appl. No. 12/244,850, filed Oct. 3, 2008.
U.S. Appl. No. 12/250,110, filed Oct. 13, 2008.
U.S. Appl. No. 12/250,171, filed Oct. 13, 2008.
U.S. Appl. No. 12/253,457, filed Oct. 17, 2008.
U.S. Appl. No. 12/277,951, filed Nov. 25, 2008.
U.S. Appl. No. 12/350,292, filed Jan. 8, 2009.
U.S. Appl. No. 12/351,633, filed Jan. 9, 2009.
U.S. Appl. No. 12/353,623, filed Jan. 14, 2009.
U.S. Appl. No. 12/353,617, filed Jan. 14, 2009.
U.S. Appl. No. 12/356,650, filed Jan. 21, 2009.
U.S. Appl. No. 12/366,298, filed Feb. 5, 2009.
U.S. Appl. No. 12/389,906, filed Feb. 20, 2009.
U.S. Appl. No. 12/389,915, filed Feb. 20, 2009.
U.S. Appl. No. 12/395,034, filed Feb. 27, 2009.
U.S. Appl. No. 12/399,222, filed Mar. 6, 2009.
U.S. Appl. No. 12/401,268, filed Mar. 10, 2009.
U.S. Appl. No. 12/413,011, filed Mar. 27, 2009.
U.S. Appl. No. 12/413,023, filed Mar. 27, 2009.
U.S. Appl. No. 12/416,583, filed Apr. 1, 2009.
U.S. Appl. No. 12/419,395, filed Apr. 7, 2009.
U.S. Appl. No. 12/423,609, filed Apr. 14, 2009.
U.S. Appl. No. 12/434,903, filed May 4, 2009.
U.S. Appl. No. 12/436,237, filed May 6, 2009.
U.S. Appl. No. 12/436,239, filed May 6, 2009.
U.S. Appl. No. 12/436,231, filed May 6, 2009.
U.S. Appl. No. 12/472,831, filed May 27, 2009.
U.S. Appl. No. 12/475,082, filed May 29, 2009.
U.S. Appl. No. 12/476,960, filed Jun. 2, 2009.
Alexander et al., "Magnetic Resonance Image-Directed Stereotactic Neurosurgery: Use of Image Fusion with Computerized Tomography to Enhance Spatial Accuracy" *Journal Neurosurgery*, 83 (1995), pp. 271-276.
Anderson et al., "A Numerical Study of Rapid Heating for High Temperature Radio Frequency Hyperthermia" *International Journal of Bio-Medical Computing*, 35 (1994), pp. 297-307.
Anonymous. (1999) Auto Suture MIBB Site Marker: Single Use Clip Applier, United States Surgical (Product instructions), 2 pages.
Anonymous. (2001) Disposable Chiba Biopsy Needles and Trays, Biopsy and Special Purpose Needles Cook Diagnostic and Interventional Products Catalog (products list), 4 pages.
Anonymous. (1987) Homer Mammalok™ Breast Lesion Needle/Wire Localizer, Namic ® Angiographic Systems Division, Glens Falls, New York, (Hospital products price list), 4 pages.
Anonymous. (1999) MIBB Site Marker, United States Surgical (Sales brochure), 4 pages.
Anonymous. Blunt Tubes with Finished Ends. Pointed Cannula, Popper & Sons Biomedical Instrument Division, (Products Price List), one page, Jul. 19, 2000.

- Anonymous. Ground Cannulae, ISPG, New Milford, CT, (Advertisement) one page, Jul. 19, 2000.
- B. Levy M.D. et al., "Update on Hysterectomy New Technologies and Techniques" OBG Management, Feb. 2003.
- B. Levy M.D., "Use of a New Vessel Ligation Device During Vaginal Hysterectomy" FIGO 2000, Washington, D.C.
- B. Levy M.D. et al., "Randomized Trial of Suture Versus Electrosurgical Bipolar Vessel Sealing in Vaginal Hysterectomy" Obstetrics & Gynecology, vol. 102, No. 1, Jul. 2003.
- B. F. Mullan et al., (May 1999) "Lung Nodules: Improved Wire for CT-Guided Localization," Radiology 211:561-565.
- B. T. Heniford M.D. et al., "Initial Research and Clinical Results with an Electrothermal Bipolar Vessel Sealer" Oct. 1999.
- Bergdahl et al., "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator" Journal of Neurosurgery 75:1 (Jul. 1991), pp. 148-151.
- Bulletin of the American Physical Society, vol. 47, No. 5, Aug. 2002, p. 41.
- C. F. Gottlieb et al., "Interstitial Microwave Hyperthermia Applicators having Submillimetre Diameters", Int. J. Hyperthermia, vol. 6, No. 3, pp. 707-714, 1990.
- C. H. Durney et al., "Antennas for Medical Applications", Antenna Handbook: Theory Application and Design, p. 24-40, Van Nostrand Reinhold, 1988 New York, V.T. Lo, S.W. Lee.
- Carbonell et al., "Comparison of the Gyrus PlasmaKinetic Sealer and the Valleylab LigaSure™ Device in the Hemostasis of Small, Medium, and Large-Sized Arteries" Carolinas Laparoscopic and Advanced Surgery Program, Carolinas Medical Center, Charlotte, NC 2003.
- Carus et al., "Initial Experience With the LigaSure™ Vessel Sealing System in Abdominal Surgery" Innovations That Work, Jun. 2002.
- Chicharo et al., "A Sliding Goertzel Algorithm" Aug. 1996 DOS pp. 283-297 Signal Processing, Elsevier Science Publishers B.V. Amsterdam, NL, vol. 52, No. 3.
- Chou, C.K., (1995) "Radiofrequency Hyperthermia in Cancer Therapy," Chapter 94 In Biologic Effects of Nonionizing Electromagnetic Fields, CRC Press, Inc., pp. 1424-1428.
- Chung et al., "Clinical Experience of Sutureless Closed Hemorrhoidectomy with LigaSure™" Diseases of the Colon & Rectum, vol. 46, No. 1, Jan. 2003.
- Cosman et al., "Radiofrequency Lesion Generation and its Effect on Tissue Impedance", Applied Neurophysiology, 51:230-242, 1988.
- Cosman et al., Theoretical Aspects of "Radiofrequency Lesions in the Dorsal Root Entry Zone" Neurosurgery 15:(1984), pp. 945-950.
- Cosman et al., "Methods of Making Nervous System Lesions" in William RH, Rengachary SS (eds): Neurosurgery, New York: McGraw•Hill, vol. 11.1, (1984), pp. 2490-2499.
- Crawford et al., "Use of the LigaSure™ Vessel Sealing System in Urologic Cancer Surger" Grand Rounds in Urology 1999, vol. 1, Issue 4, pp. 10-17.
- Dulemba et al., "Use of a Bipolar Electrothermal Vessel Sealer in Laparoscopically Assisted Vaginal Hysterectomy" Sales/Product Literature; Jan. 2004.
- E. David Crawford, "Evaluation of a New Vessel Sealing Device in Urologic Cancer Surgery" Sales/Product Literature 2000.
- E. David Crawford, "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Venous Complex" Sales/Product Literature 2000.
- Esterline Product Literature, "Light Key: Visualize a Virtual Keyboard. One With No Moving Parts", 4 pages.
- Esterline, "Light Key Projection Keyboard" 2004 Advanced Input Systems, located at: <<http://www.advanced-input.com/lightkey>> last visited on Feb. 10, 2005.
- Geddes et al., "The Measurement of Physiologic Events by Electrical Impedance" Am. J. MI, Jan. Mar. 1964, pp. 16-27.
- Goldberg et al., "Image-guided Radiofrequency Tumor Ablation: Challenges and Opportunities - Part I", (2001) J Vase. Interv. Radiol, vol. 12, pp. 1021-1032.
- Goldberg et al., "Tissue Ablation with Radiofrequency: Effect of Probe Size, Gauge, Duration, and Temperature on Lesion Volume" Acad Radio (1995) vol. 2, No. 5, pp. 399-404.
- Heniford et al., "Initial Results with an Electrothermal Bipolar Vessel Sealer" Surgical Endoscopy (2001) 15:799- 801.
- Herman et al., "Laparoscopic Intestinal Resection With the LigaSure™ Vessel Sealing System: A Case Report" Innovations That Work, Feb. 2002.
- Ian D. McRury et al., The Effect of Ablation Sequence and Duration on Lesion Shape Using Rapidly Pulsed Radiofrequency Energy Through Electrodes, Feb. 2000, Springer Netherlands, vol. 4; No. 1, pp. 307-320.
- Johnson et al., "Evaluation of a Bipolar Electrothermal Vessel Sealing Device in Hemorrhoidectomy" Sales/Product Literature, Jan. 2004.
- Jarrett et al., "Use of the LigaSure™ Vessel Sealing System for Peri-Hilar Vessels in Laparoscopic Nephrectomy" Sales/Product Literature 2000.
- Johnson, "Evaluation of the LigaSure™ Vessel Sealing System in Hemorrhoidectomy" American College of Surgeons (ACS) Clinic La Congress Poster (2000).
- Johnson, "Use of the LigaSure™ Vessel Sealing System in Bloodless Hemorrhoidectomy" Innovations That Work, Mar. 2000.
- Joseph G. Andriole M.D. et al., "Biopsy Needle Characteristics Assessed in the Laboratory", Radiology 148:659- 662, Sep. 1983.
- Joseph Ortenberg, " LigaSure™ System Used in Laparoscopic 1st and 2nd Stage Orchiopexy" Innovations That Work, Nov. 2002.
- K. Ogata, Modern Control Engineering, Prentice-Hall, Englewood Cliffs, N.J., 1970.
- Kennedy et al., "High-burst-strength, feedback-controlled bipolar vessel sealing" Surgical Endoscopy (1998) 12: 876-878.
- Kopans, D.B. et al., (Nov. 1985) "Spring Hookwire Breast Lesion Localizer: Use with Rigid-Compression. Mammographic Systems," Radiology 157(2):537-538.
- Koyle et al., "Laparoscopic Palomo Varicocele Ligation in Children and Adolescents" Pediatric Endosurgery & Innovative Techniques, vol. 6, No. 1, 2002.
- LigaSure™ Vessel Sealing System, the Seal of Confidence in General, Gynecologic, Urologic, and Laparoscopic Surgery, Sales/Product Literature, Jan. 2004.
- Livraghi et al., (1995) "Saline-enhanced RF Tissue Ablation in the Treatment of Liver Metastases", Radiology, pp. 205-210.
- Lyndon B. Johnson Space Center, Houston, Texas, "Compact Directional Microwave Antenna for Localized Heating," Nasa Tech Briefs, Mar. 2008.
- M. A. Astrahan, "A Localized Current Field Hyperthermia System for Use with 192-Iridium Interstitial Implants" Medical Physics. 9(3), May/June. 1982.
- Magdy F. Iskander et al., "Design Optimization of Interstitial Antennas", IEEE Transactions on Biomedical Engineering, vol. 36, No. 2, Feb. 1989, pp. 238-246.
- McGahan et al., (1995) "Percutaneous Ultrasound-guided Radiofrequency Electrocautery Ablation of Prostate Tissue in Dogs", Acad Radiol, vol. 2, No. 1: pp. 61-65.
- McLellan et al., "Vessel Sealing for Hemostasis During Pelvic Surgery" Int'l Federation of Gynecology and Obstetrics FIGO World Congress 2000, Washington, DC.
- MDTECH product literature (Mar. 2000) I'D Wire: product description, 1 page.
- MDTECH product literature (Dec. 1999) "FlexStrand": product description, 1 page.
- Medtrex Brochure "The O.R. Pro 300" 1 page, Sep. 1998.
- Michael Choti, "Abdominoperineal Resection with the LigaSure™ Vessel Sealing System and LigaSure™ Atlas 20 cm Open Instrument" Innovations That Work, Jun. 2003.
- Muller et al., "Extended Left Hemicolectomy Using the LigaSure™ Vessel Sealing System" Innovations That Work. LJ, Sep. 1999.
- Murakami, R. et al., (1995). "Treatment of Hepatocellular Carcinoma: Value of Percutaneous Microwave Coagulation," American Journal of Radiology (AJR) 164:1159-1164.
- Ni Wei et al., "A Signal Processing Method for the Coriolis Mass Flowmeter Based on a Normalized . . ." Journal of Applied Sciences•Yingyong Kexue Xuebao, Shangha CN, vol. 23, No. 2:(2005.03); pp. 160-184.
- Ogden, "Goertzel Alternative to the Fourier Transform" Jun. 1993 pp. 485-487 Electronics World; Reed Business Publishing, Sutton, Surrey, BG, vol. 99, No. 9, 1687.

- Olsson M.D. et al., "Radical Cystectomy in Females" *Current Surgical Techniques in Urology*, vol. 14, Issue 3, 2001.
- Organ, L. W., "Electrophysiologic Principles of Radiofrequency Lesion Making" *Appl. Neurophysiol.*, vol. 39: pp. 69-76 (1976/77).
- P.R. Stauffer et al., "Interstitial Heating Technologies", *Thermoradiotherapy and Thermochemotherapy (1995)* vol. I, *Biology, Physiology, Physics*, pp. 279-320.
- Palazzo et al., "Randomized clinical trial of LigaSure™ versus open haemorrhoidectomy" *British Journal of Surgery* 2002,89,154-157 "Innovations in Electrosurgery" Sales/Product Literature; Dec. 31, 2000.
- Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" *The American Journal of Surgery*, vol. 181, No. 3, Apr. 2001, pp. 236-237.
- Peterson et al., "Comparison of Healing Process Following Ligation with Sutures and Bipolar Vessel Sealing" *Surgical Technology International* (2001).
- R. Gennari et al., (Jun. 2000) "Use of Technetium-99m-Labeled Colloid Albumin for Preoperative and Intraoperative Localization of Non palpable Breast Lesions," *American College of Surgeons*. 190(6):692-699.
- Valleylab Brochure, "Reducing Needlestick Injuries in the Operating Room" 1 page, Mar. 2001.
- Reidenbach, (1995) "First Experimental Results with Special Applicators for High-Frequency Interstitial Thermoablation", *Society Minimally Invasive Therapy*, 4(Suppl 1):40 (Abstr).
- Richard Wolf Medical Instruments Corp. Brochure, "Kleppinger Bipolar Forceps & Bipolar Generator" 3 pages, Jan. 1989.
- Rothenberg et al., "Use of the LigaSure™ Vessel Sealing System in Minimally Invasive Surgery in Children" *Int'l Pediatric Endosurgery Group (I PEG)* 2000.
- Sayfan et al., "Sutureless Closed Hemorrhoidectomy: A New Technique" *Annals of Surgery*, vol. 234, No. 1, Jul. 2001, pp. 21-24.
- Sengupta et al., "Use of a Computer-Controlled Bipolar Diathermy System in Radical Prostatectomies and Other Open Urological Surgery" *ANZ Journal of Surgery* (2001)71.9 pp. 538-540.
- Sigel et al., "The Mechanism of Blood Vessel Closure by High Frequency Electrocoagulation" *Surgery Gynecology & Obstetrics*, Oct. 1965 pp. 823-831.
- Solbiati et al., (2001) "Percutaneous Radio-frequency Ablation of Hepatic Metastases from Colorectal Cancer: Long-term Results in 117 Patients", *Radiology*, vol. 221, pp. 159-166.
- Strasberg et al., "Use of a Bipolar Vessel-Sealing Device for Parenchymal Transection During Liver Surgery" *Journal of Gastrointestinal Surgery*, vol. 6, No. 4, Jul./Aug. 2002 pp. 569-574.
- Stuart W. Young, *Nuclear Magnetic Resonance Imaging—Basic Principles*, Raven Press, New York, 1984.
- Sugita et al., "Bipolar Coagulator with Automatic Thermocontrol" *J. Neurosurg.*, vol. 41, Dec. 1944, pp. 777-779.
- Sylvain Labonte et al., "Monopole Antennas for Microwave Catheter Ablation", *IEEE Trans. On Microwave Theory and Techniques*, vol. 44, No. 10, pp. 1832-1840, Oct. 1995.
- T. Matsukawa et al., "Percutaneous Microwave Coagulation Therapy in Liver Tumors", *Acta Radiologica*, vol. 38, pp. 410-415, 1997.
- T. Seki et al., (1994) "Ultrasonically Guided Percutaneous Microwave Coagulation Therapy for Small Hepatocellular Carcinoma," *Cancer* 74(3):817-825.
- S. Humphries Jr. et al., "Finite Element Codes to Model Electrical Heating and Non-Linear Thermal Transport in Biological Media", *Proc. ASME HTD-355*, 131 (1997).
- Urologix, Inc.-Medical Professionals: Targis™ Technology (Date Unknown). "Overcoming the Challenge" located at: <<http://www.urologix.com/medicaUtechnology.html>> last visited on Apr. 27, 2001, 3 pages.
- Urrutia et al., (1988). "Retractable-Barb Needle for Breast Lesion Localization: Use in 60 Cases," *Radiology* 169(3):845-847.
- Valleylab Brochure, "Valleylab Electroshield Monitoring System" 2 pages, Nov. 1995.
- ValleyLab Brochure, "Electrosurgery: A Historical Overview", *Innovations in Electrosurgery*, 1999.
- Vallfors et al., "Automatically Controlled Bipolar Electrocoagulation-'COA-COMP'" *Neurosurgical Review* 7:2-3 (1984) pp. 187-190.
- W. Scott Helton, "LigaSure™ Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery" Sales/Product Literature 1999.
- Wald et al., "Accidental Burns", *JAMA*, Aug. 16, 1971, vol. 217, No. 7, pp. 916-921.
- Walt Boyles, "Instrumentation Reference Book", 2002, Butterworth-Heinemann, pp. 262-264.
- European Search Report EP 03721482 dated Feb. 6, 2006.
- European Search Report EP 04009964 dated Jul. 28, 2004.
- European Search Report EP 04013772 dated Apr. 11, 2005.
- European Search Report EP 04015980 dated Nov. 3, 2004.
- European Search Report EP 04015981.6 dated Oct. 25, 2004.
- European Search Report EP 04027314 dated Mar. 31, 2005.
- European Search Report EP 04027479 dated Mar. 17, 2005.
- European Search Report EP 04027705 dated Feb. 10, 2005.
- European Search Report EP 04710258 dated Oct. 15, 2004.
- European Search Report EP 04752343.6 dated Jul. 31, 2007.
- European Search Report EP 05002027.0 dated May 12, 2005.
- European Search Report EP 05002769.7 dated Jun. 19, 2006.
- European Search Report EP 05013463.4 dated Oct. 7, 2005.
- European Search Report EP 05013895 dated Oct. 21, 2005.
- European Search Report EP 05014156.3 dated Jan. 4, 2006.
- European Search Report EP 05016399 dated Jan. 13, 2006.
- European Search Report EP 05017281 dated Nov. 24, 2005.
- European Search Report EP 05019130.3 dated Oct. 27, 2005.
- European Search Report EP 05019882 dated Feb. 16, 2006.
- European Search Report EP 05020665.5 dated Feb. 27, 2006.
- European Search Report EP 05020666.3 dated Feb. 27, 2006.
- European Search Report EP 05021025.1 dated Mar. 13, 2006.
- European Search Report EP 05021197.8 dated Feb. 20, 2006.
- European Search Report EP 05021777 dated Feb. 23, 2006.
- European Search Report EP 05021779.3 dated Feb. 2, 2006.
- European Search Report EP 05021780.1 dated Feb. 23, 2006.
- European Search Report EP 05021935 dated Jan. 27, 2006.
- European Search Report EP 05021936.9 dated Feb. 6, 2006.
- European Search Report EP 05021937.7 dated Jan. 23, 2006.
- European Search Report EP 05021939 dated Jan. 27, 2006.
- European Search Report EP 05021944.3 dated Jan. 25, 2006.
- European Search Report EP 05022350.2 dated Jan. 30, 2006.
- European Search Report EP 05023017.6 dated Feb. 24, 2006.
- European Search Report EP 05025423.4 dated Jan. 19, 2007.
- European Search Report EP 05025424 dated Jan. 30, 2007.
- European Search Report EP 06000708.5 dated May 15, 2006.
- European Search Report EP 06002279.5 dated Mar. 30, 2006.
- European Search Report EP 06005185.1 dated May 10, 2006.
- European Search Report EP 06005540 dated Sep. 24, 2007.
- European Search Report EP 06006717.0 dated Aug. 11, 2006.
- European Search Report EP 06006961 dated Oct. 22, 2007.
- European Search Report EP 06006963 dated Jul. 25, 2006.
- European Search Report EP 06008779.8 dated Jul. 13, 2006.
- European Search Report EP 06009435 dated Jul. 13, 2006.
- European Search Report EP 06010499.9 dated Jan. 29, 2008.
- European Search Report EP 06014461.5 dated Oct. 31, 2006.
- European Search Report EP 06018206.0 dated Oct. 20, 2006.
- European Search Report EP 06019768 dated Jan. 17, 2007.
- European Search Report EP 06020574.7 dated Oct. 2, 2007.
- European Search Report EP 06020583.8 dated Feb. 7, 2007.
- European Search Report EP 06020584.6 dated Feb. 1, 2007.
- European Search Report EP 06020756.0 dated Feb. 16, 2007.
- European Search Report EP 06022028.2 dated Feb. 13, 2007.
- European Search Report EP 06023756.7 dated Feb. 21, 2008.
- European Search Report EP 06024122.1 dated Apr. 16, 2007.
- European Search Report EP 06024123.9 dated Mar. 6, 2007.
- European Search Report EP 06025700.3 dated Apr. 12, 2007.
- European Search Report EP 07000885.9 dated May 15, 2007.
- European Search Report EP 07001480.8 dated Apr. 19, 2007.
- European Search Report EP 07001481.6 dated May 2, 2007.
- European Search Report EP 07001485.7 dated May 23, 2007.
- European Search Report EP 07001488.1 dated Jun. 5, 2007.
- European Search Report EP 07001489.9 dated Dec. 20, 2007.
- European Search Report EP 07001491 dated Jun. 6, 2007.
- European Search Report EP 07001527.6 dated May 18, 2007.
- European Search Report EP 07007783.9 dated Aug. 14, 2007.

European Search Report EP 07008207.8 dated Sep. 13, 2007.
European Search Report EP 07009026.1 dated Oct. 8, 2007.
European Search Report EP 07009028 dated Jul. 16, 2007.
European Search Report EP 07009029.5 dated Jul. 20, 2007.
European Search Report EP 07009321.6 dated Aug. 28, 2007.
European Search Report EP 07009322.4 dated Jan. 14, 2008.
European Search Report EP 07010672.9 dated Oct. 16, 2007.
European Search Report EP 07010673.7 dated Oct. 5, 2007.
European Search Report EP 07013779.9 dated Oct. 26, 2007.
European Search Report EP 07015191.5 dated Jan. 23, 2007.
European Search Report EP 07015601.3 dated Jan. 4, 2007.
European Search Report EP 07015602.1 dated Dec. 20, 2007.
European Search Report EP 07018375.1 dated Jan. 8, 2008.
European Search Report EP 07018821 dated Jan. 14, 2008.
European Search Report EP 07019173.9 dated Feb. 12, 2008.
European Search Report EP 07019174.7 dated Jan. 29, 2008.
European Search Report EP 07019178.8 dated Feb. 12, 2008.
European Search Report EP 07020283.3 dated Feb. 5, 2008.
European Search Report EP 07253835.8 dated Dec. 20, 2007.
European Search Report EP 08001019 dated Sep. 23, 2008.
European Search Report EP 08004975 dated Jul. 24, 2008.
European Search Report EP 08006731.7 dated Jul. 29, 2008.
European Search Report EP 08006733 dated Jul. 7, 2008.
European Search Report EP 08006734.1 dated Aug. 18, 2008.

European Search Report EP 08006735.8 dated Jan. 8, 2009.
European Search Report EP 08015842 dated Dec. 5, 2008.
European Search Report EP 98300964.8 dated Dec. 13, 2000.
European Search Report EP 98944778 dated Nov. 7, 2000.
European Search Report EP 98958575.7 dated Oct. 29, 2002.
International Search Report PCT/US01/11218 dated Aug. 14, 2001.
International Search Report PCT/US01/11224 dated Nov. 13, 2001.
International Search Report PCT/US01/11340 dated Aug. 16, 2001.
International Search Report PCT/US01/11420 dated Oct. 16, 2001.
International Search Report PCT/US02/01890 dated Jul. 25, 2002.
International Search Report PCT/US02/11100 dated Jul. 16, 2002.
International Search Report PCT/US03/09483 dated Aug. 13, 2003.
International Search Report PCT/US03/22900 dated Dec. 2, 2003.
International Search Report PCT/US03/37110 dated Jul. 25, 2005.
International Search Report PCT/US03/37111 dated Jul. 28, 2004.
International Search Report PCT/US03/37310 dated Aug. 13, 2004.
International Search Report PCT/US04/04685 dated Aug. 27, 2004.
International Search Report PCT/US04/13273 dated Dec. 15, 2004.
International Search Report PCT/US04/15311 dated Jan. 12, 2004.
International Search Report PCT/US98/18640 dated Jan. 29, 1998.
International Search Report PCT/US98/23950 dated Jan. 14, 1998.
International Search Report PCT/US99/24869 dated Feb. 11, 2000.

* cited by examiner

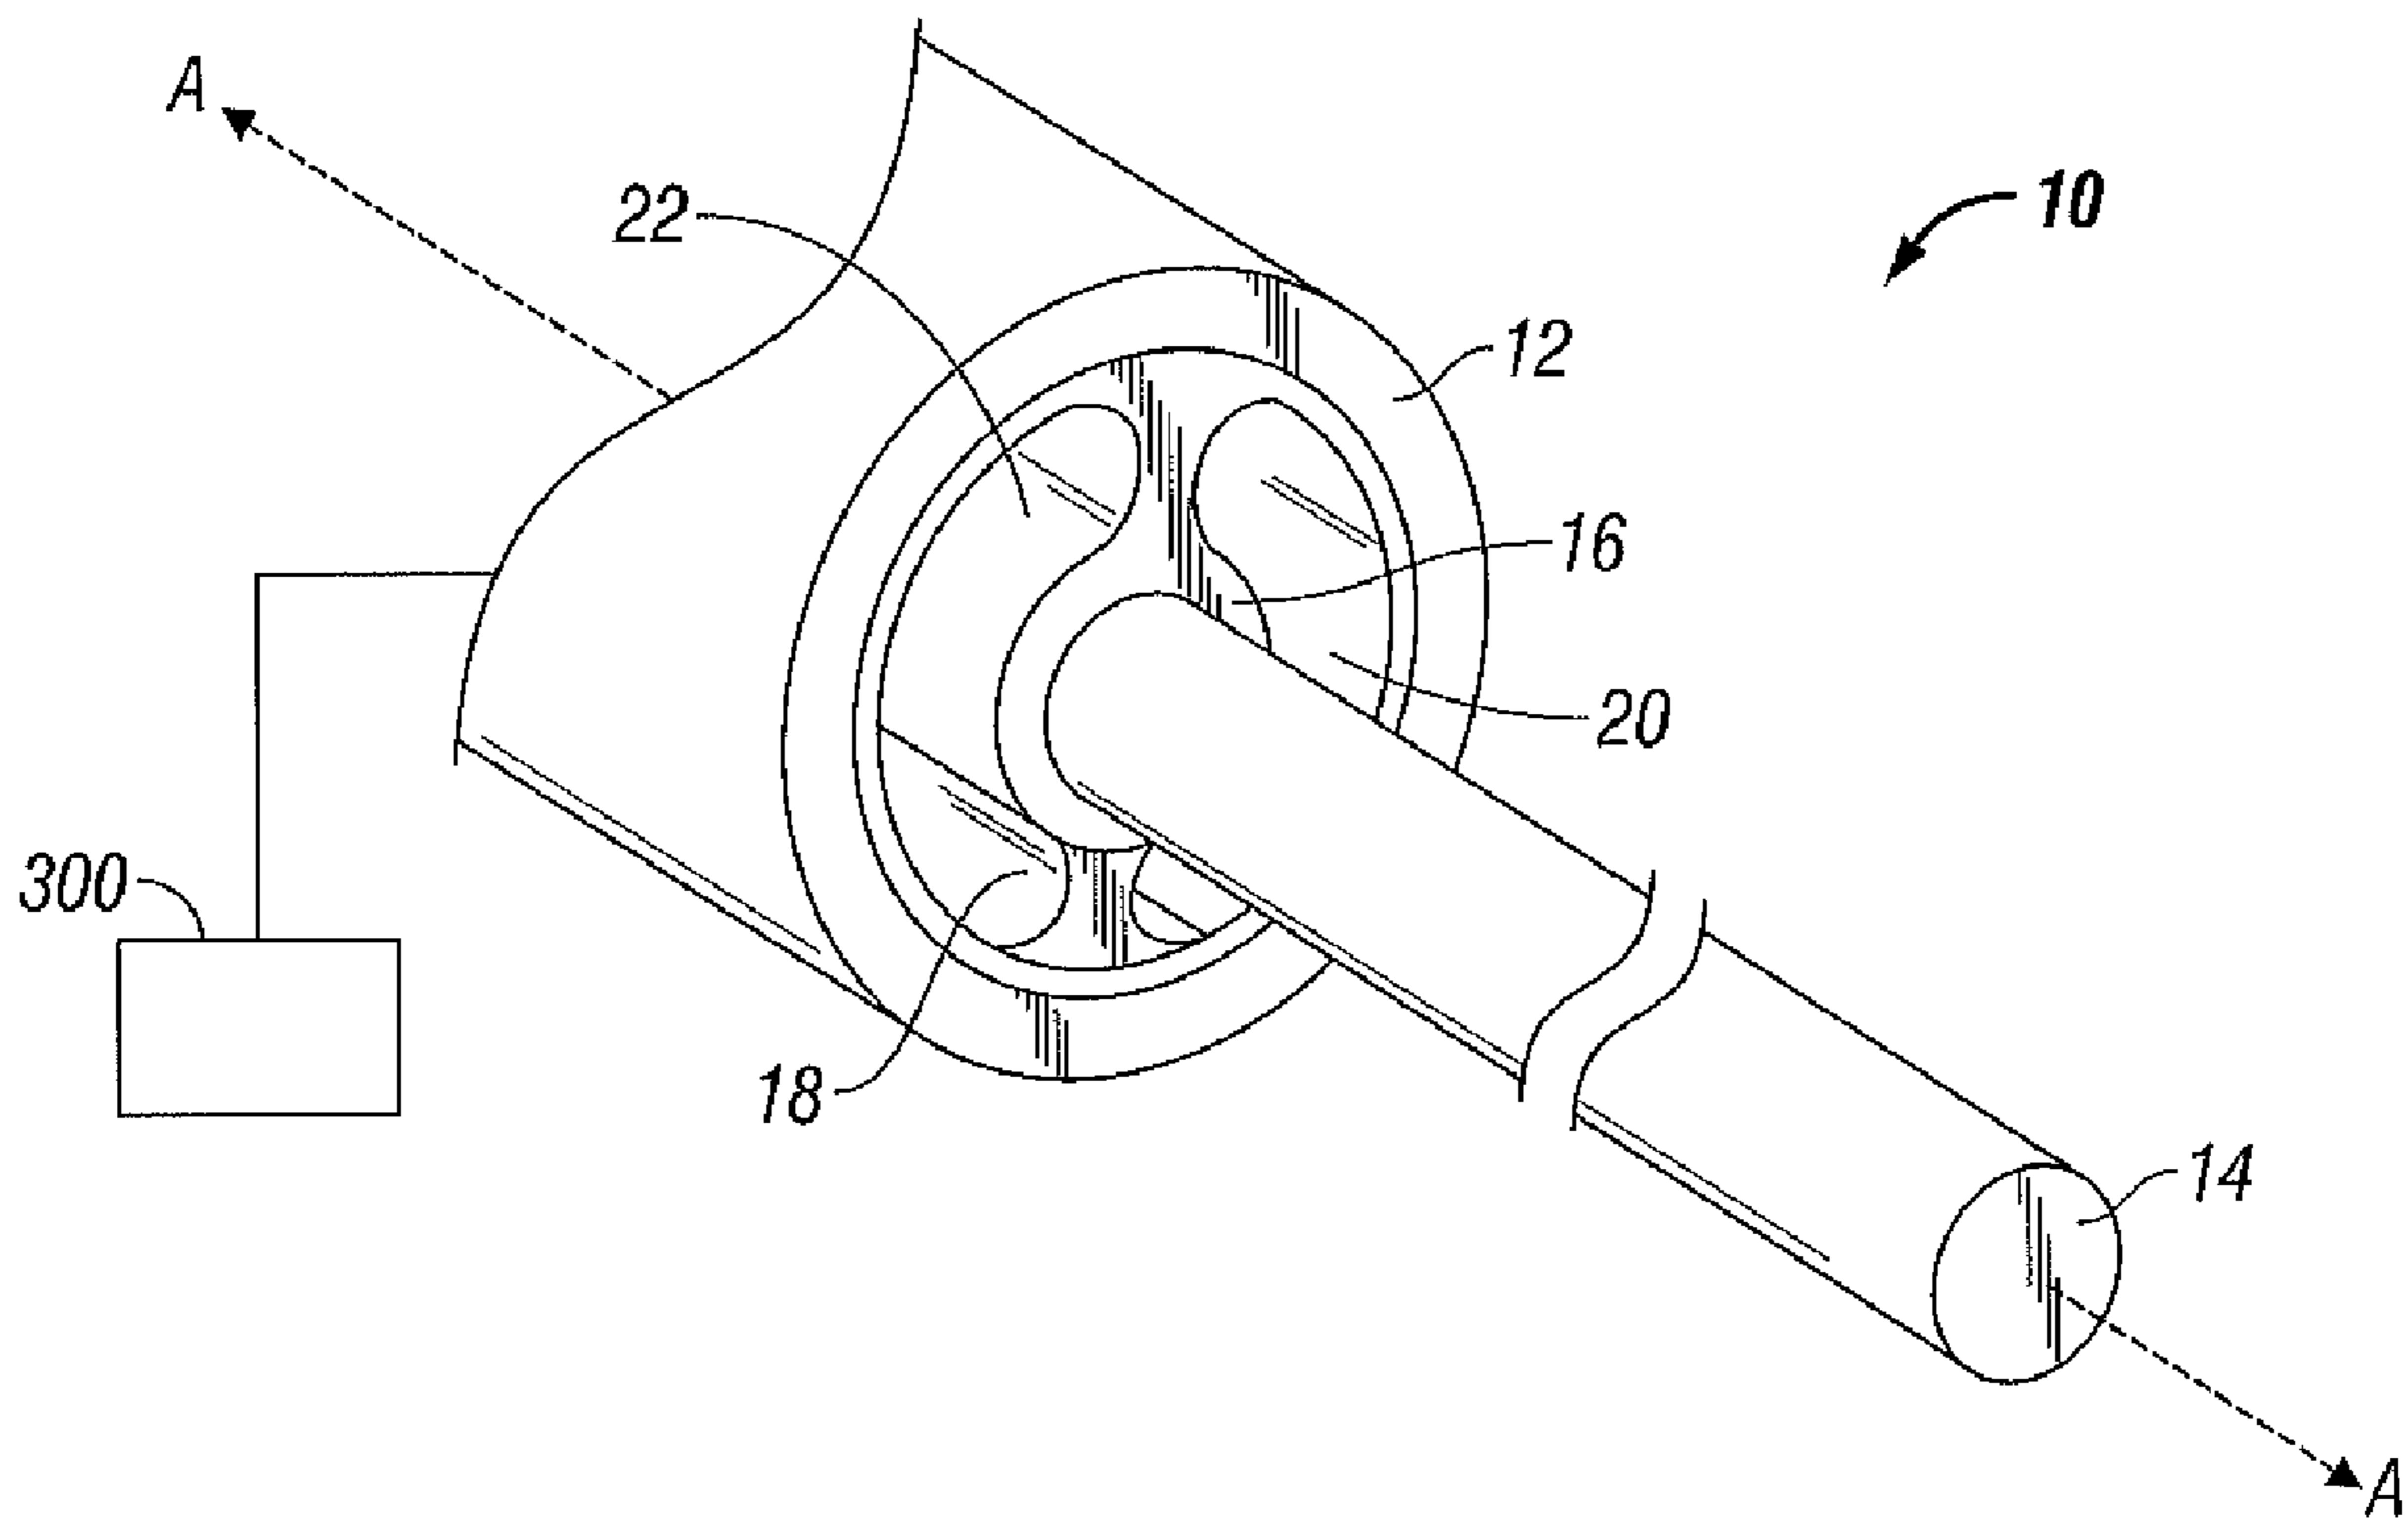


FIG. 1A

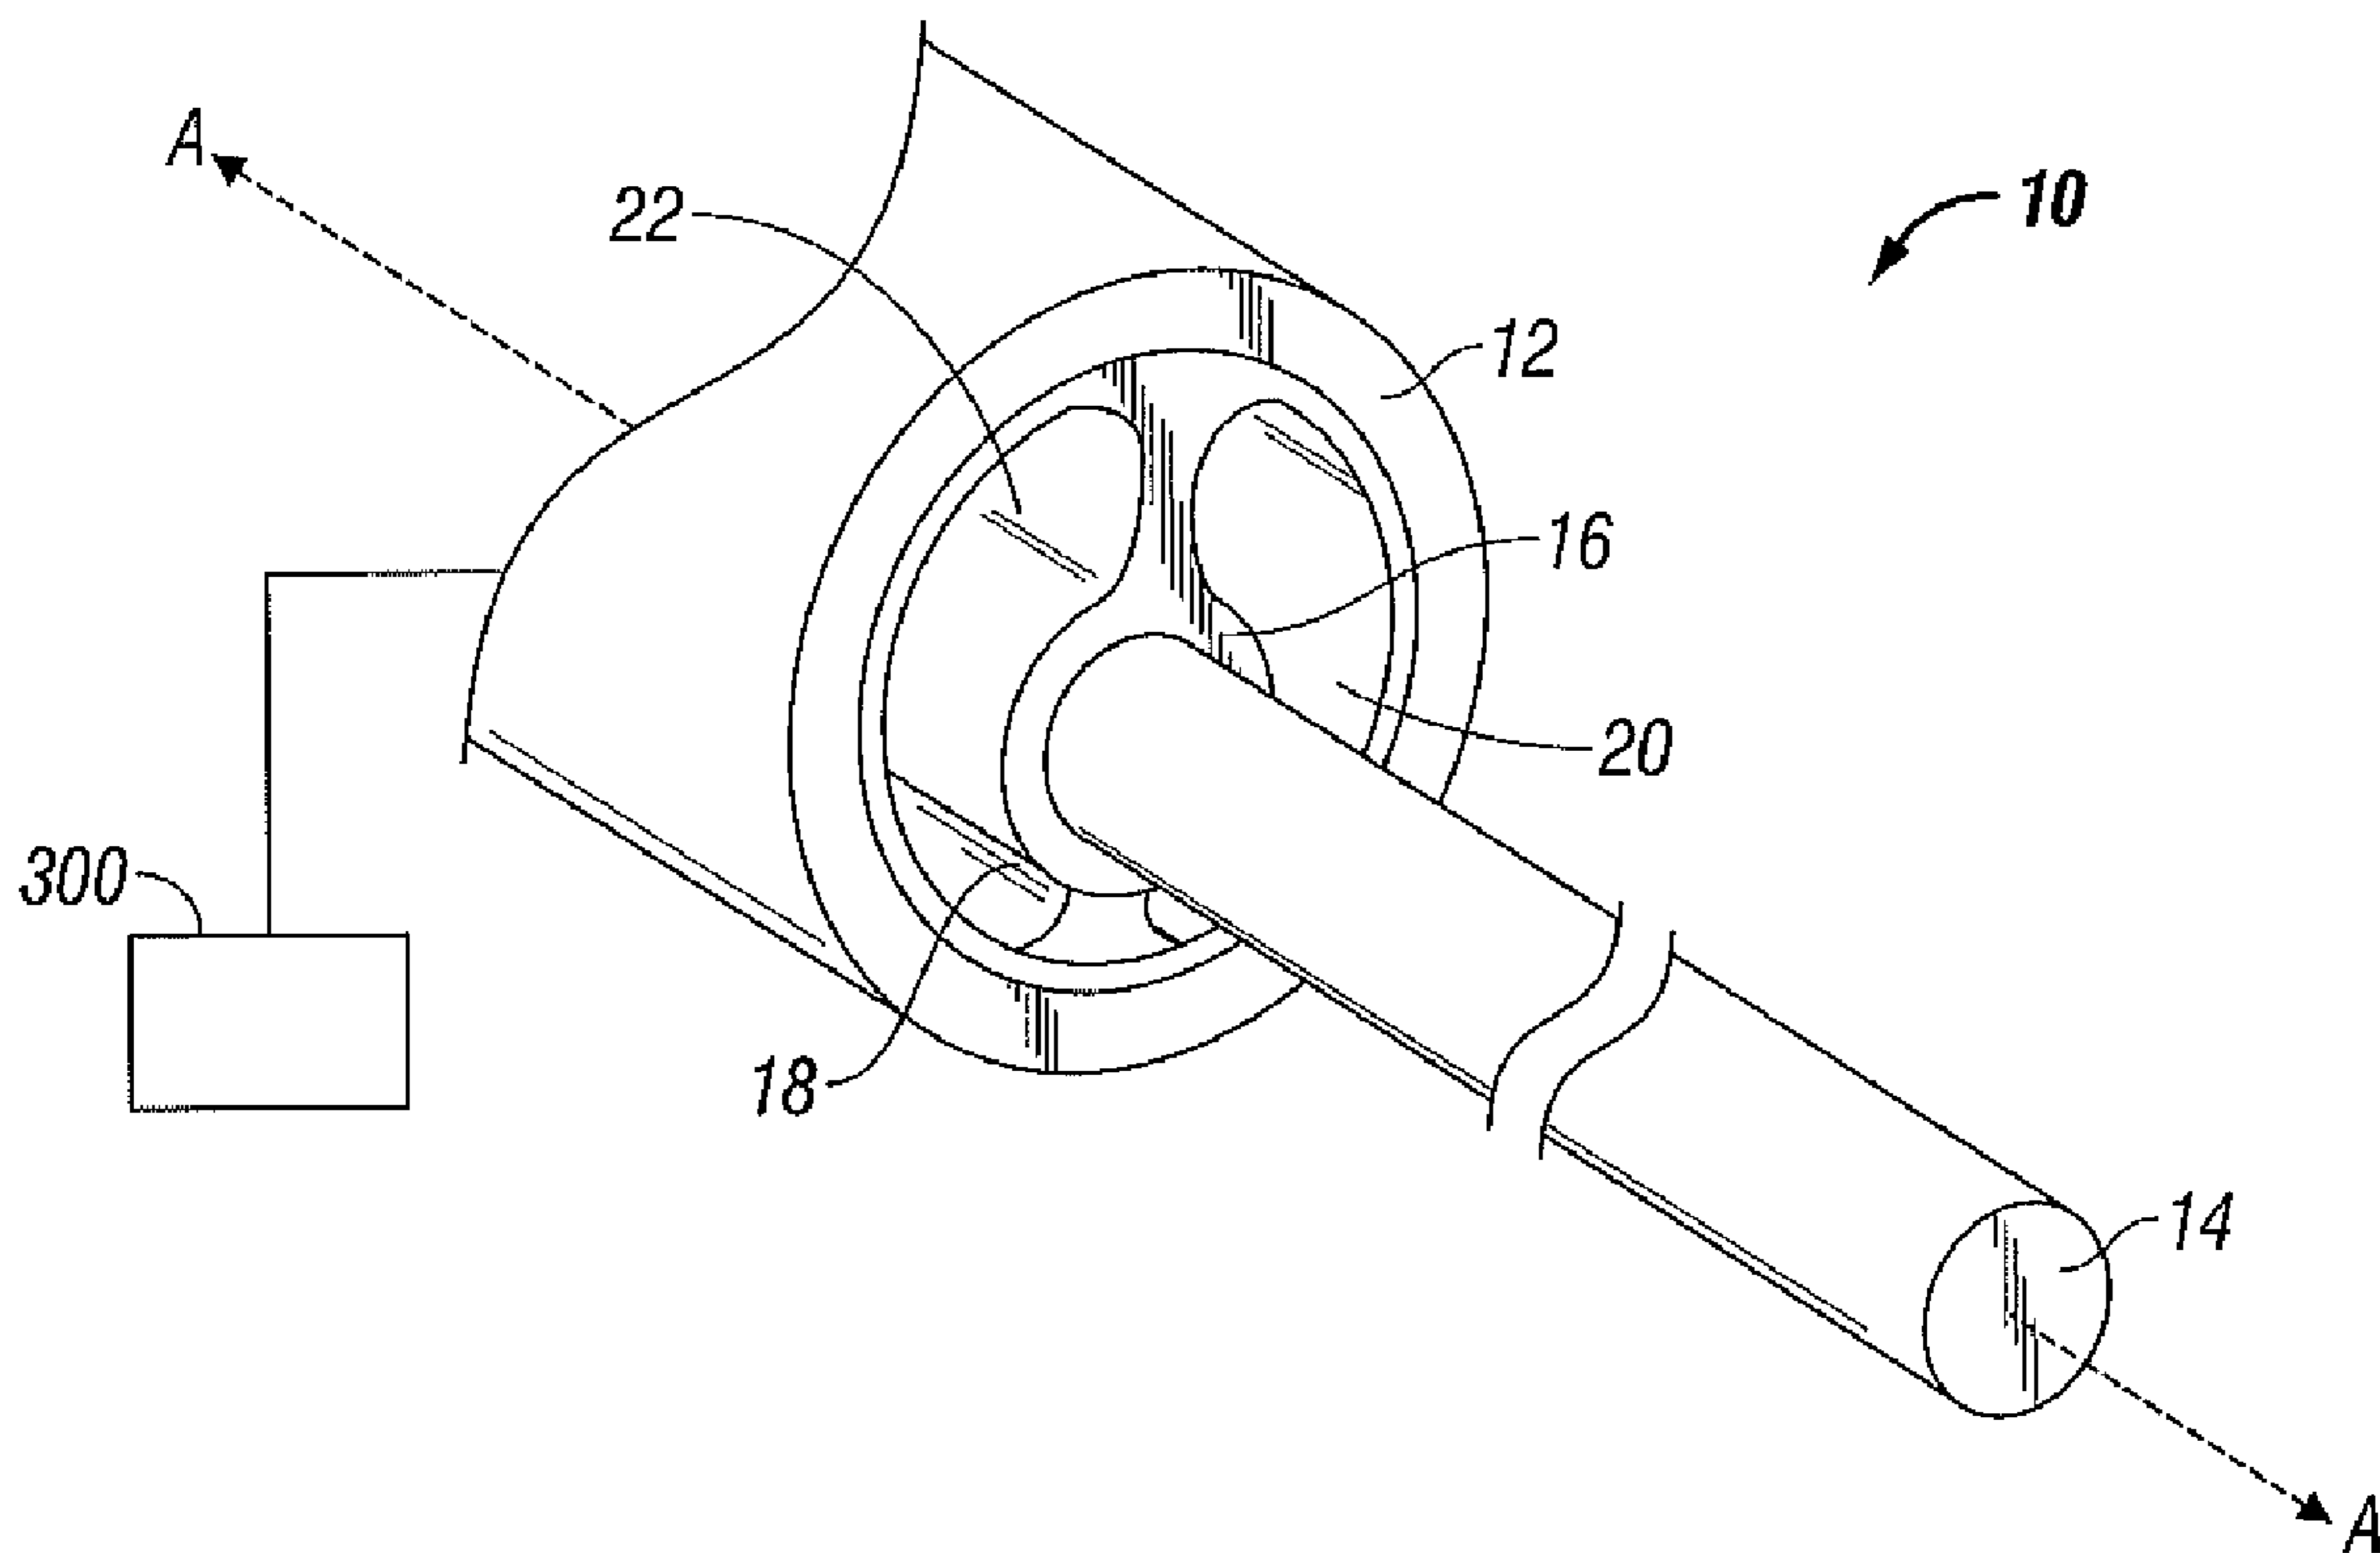


FIG. 1B

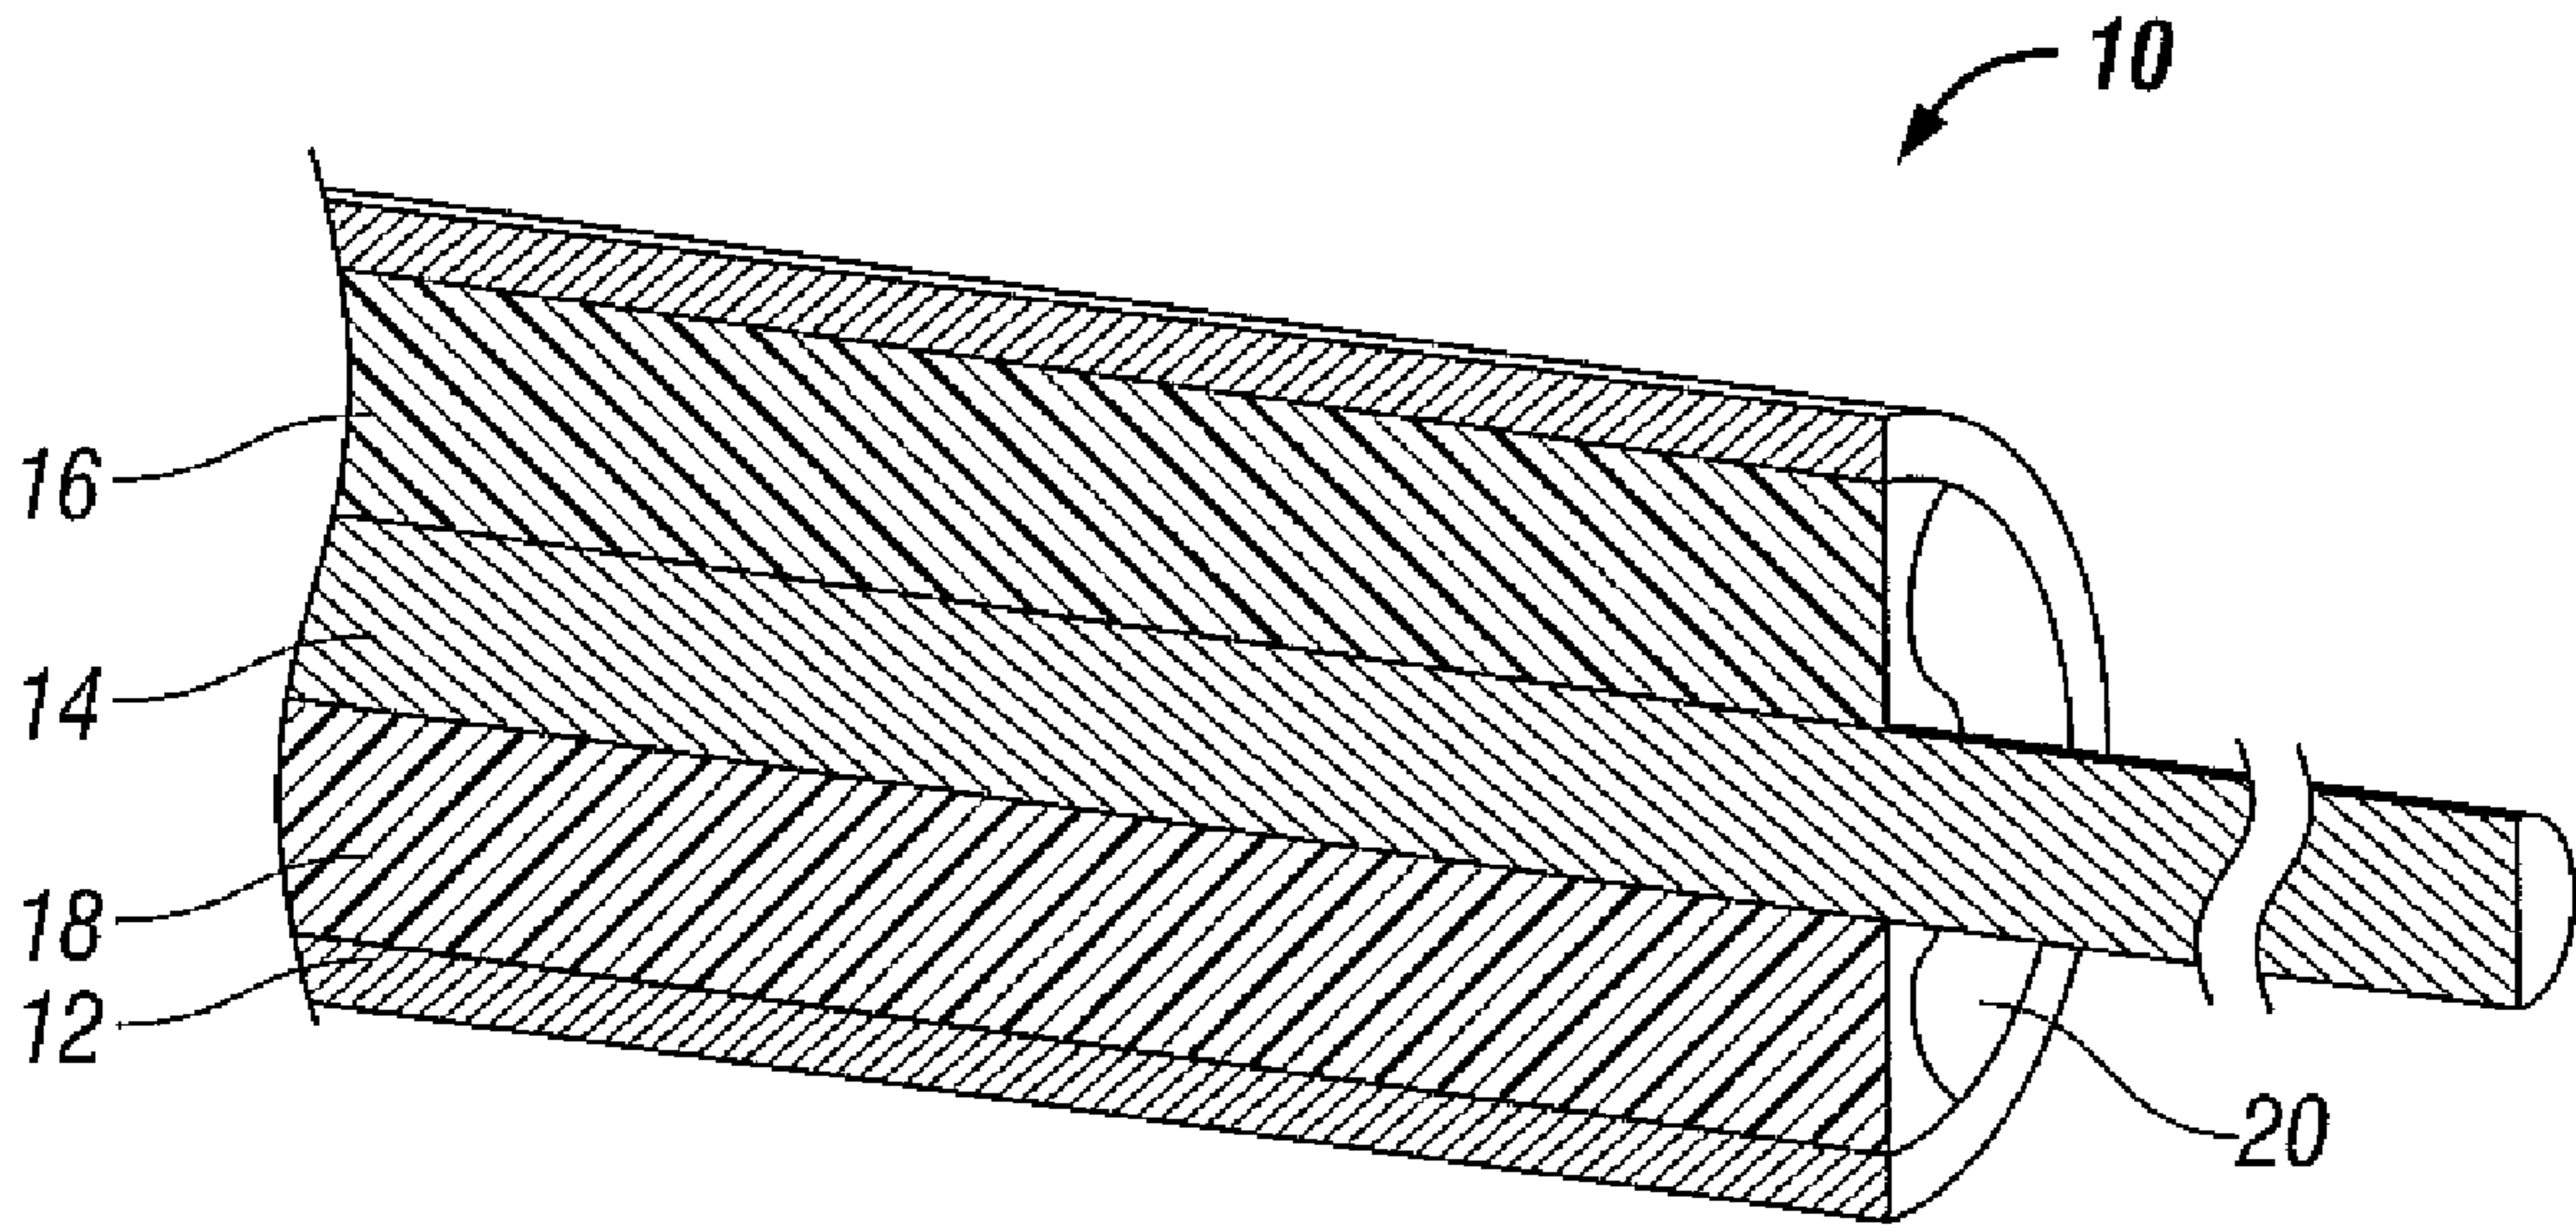


FIG. 1C

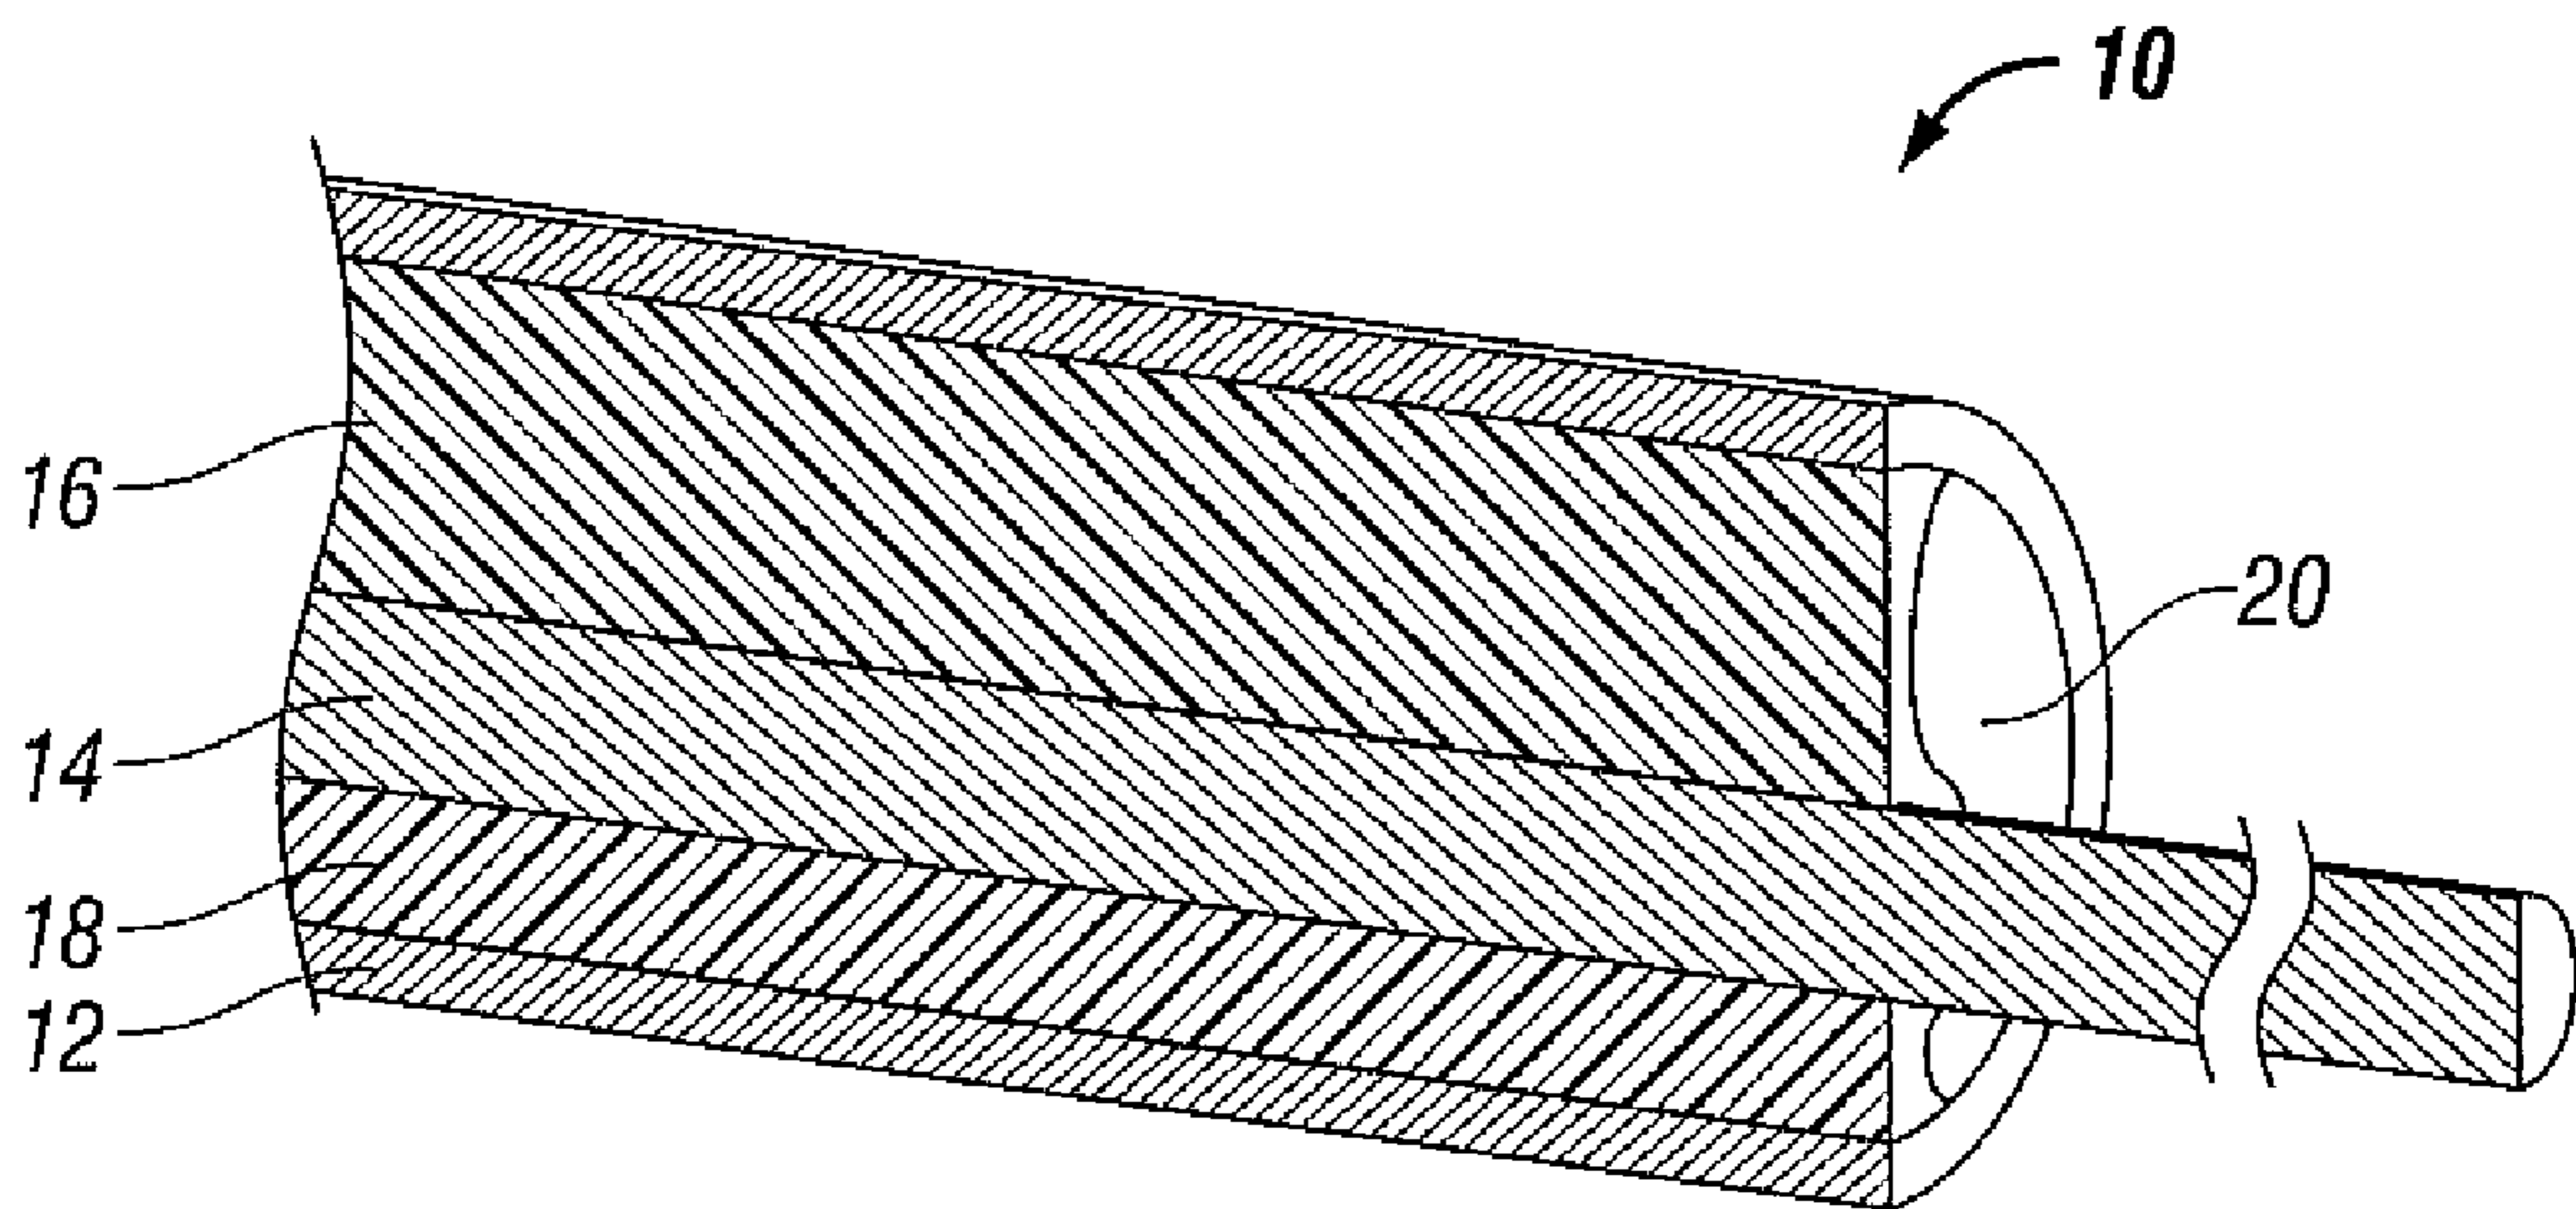


FIG. 1D

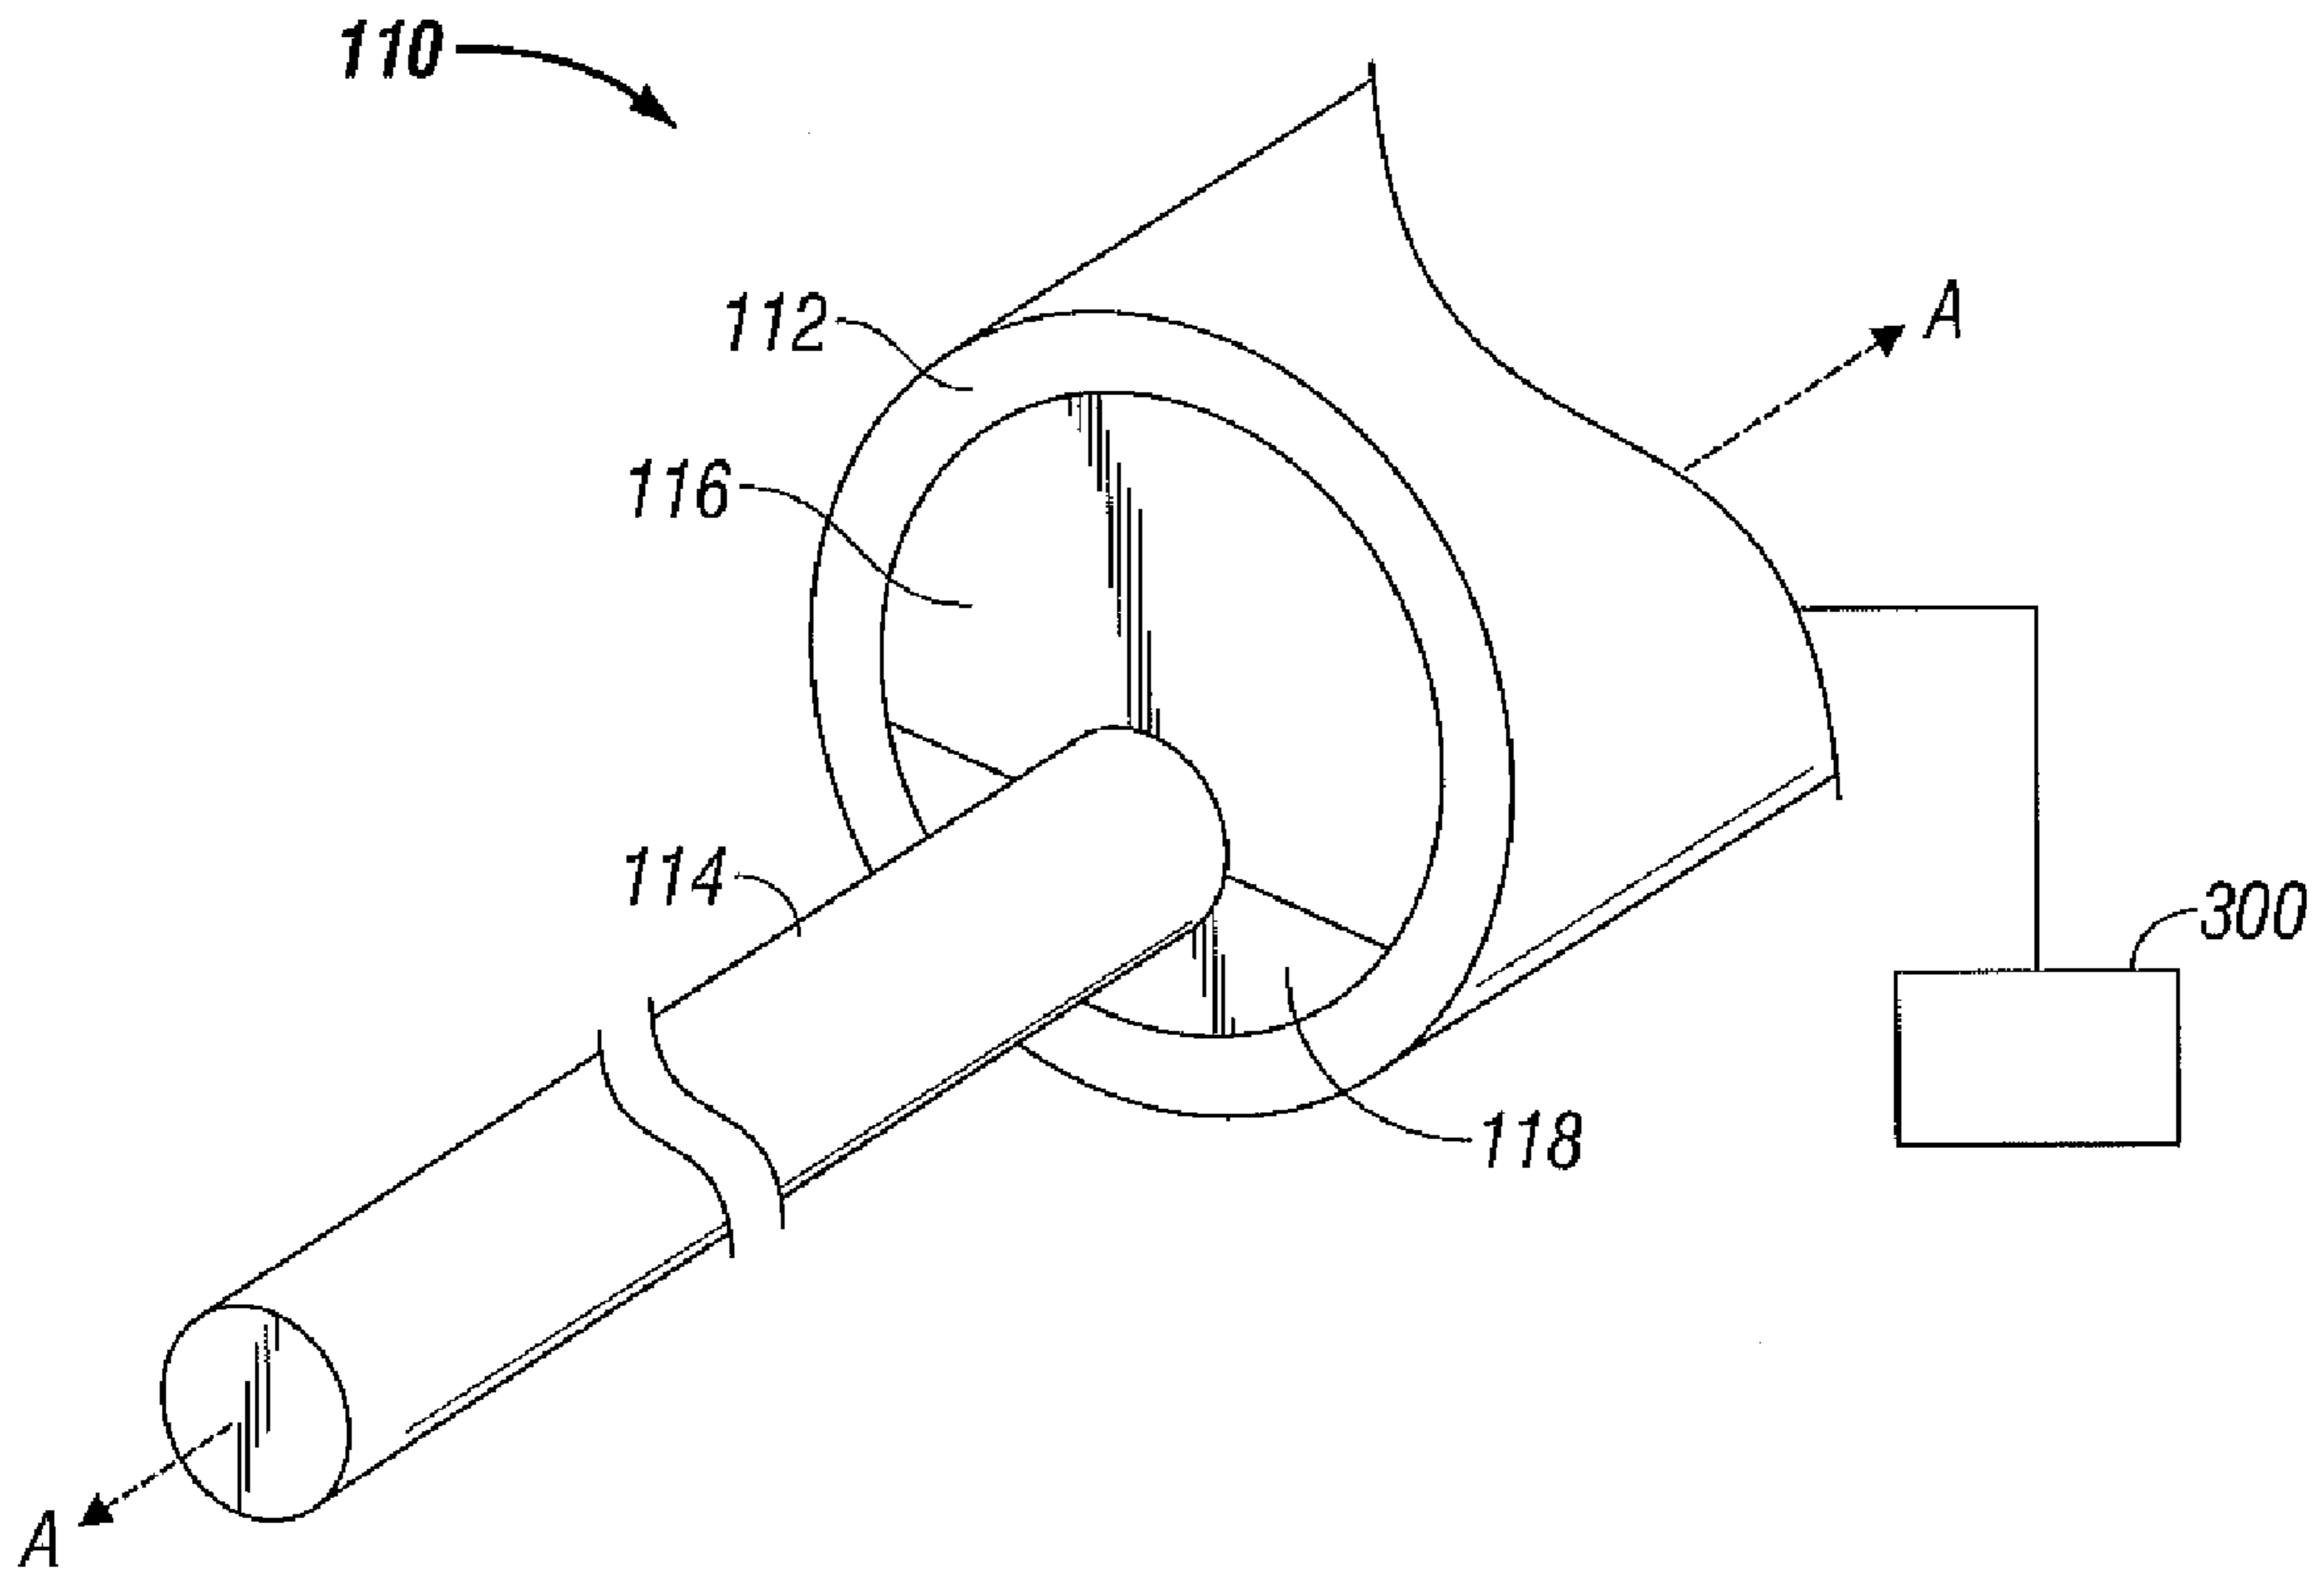


FIG. 2A

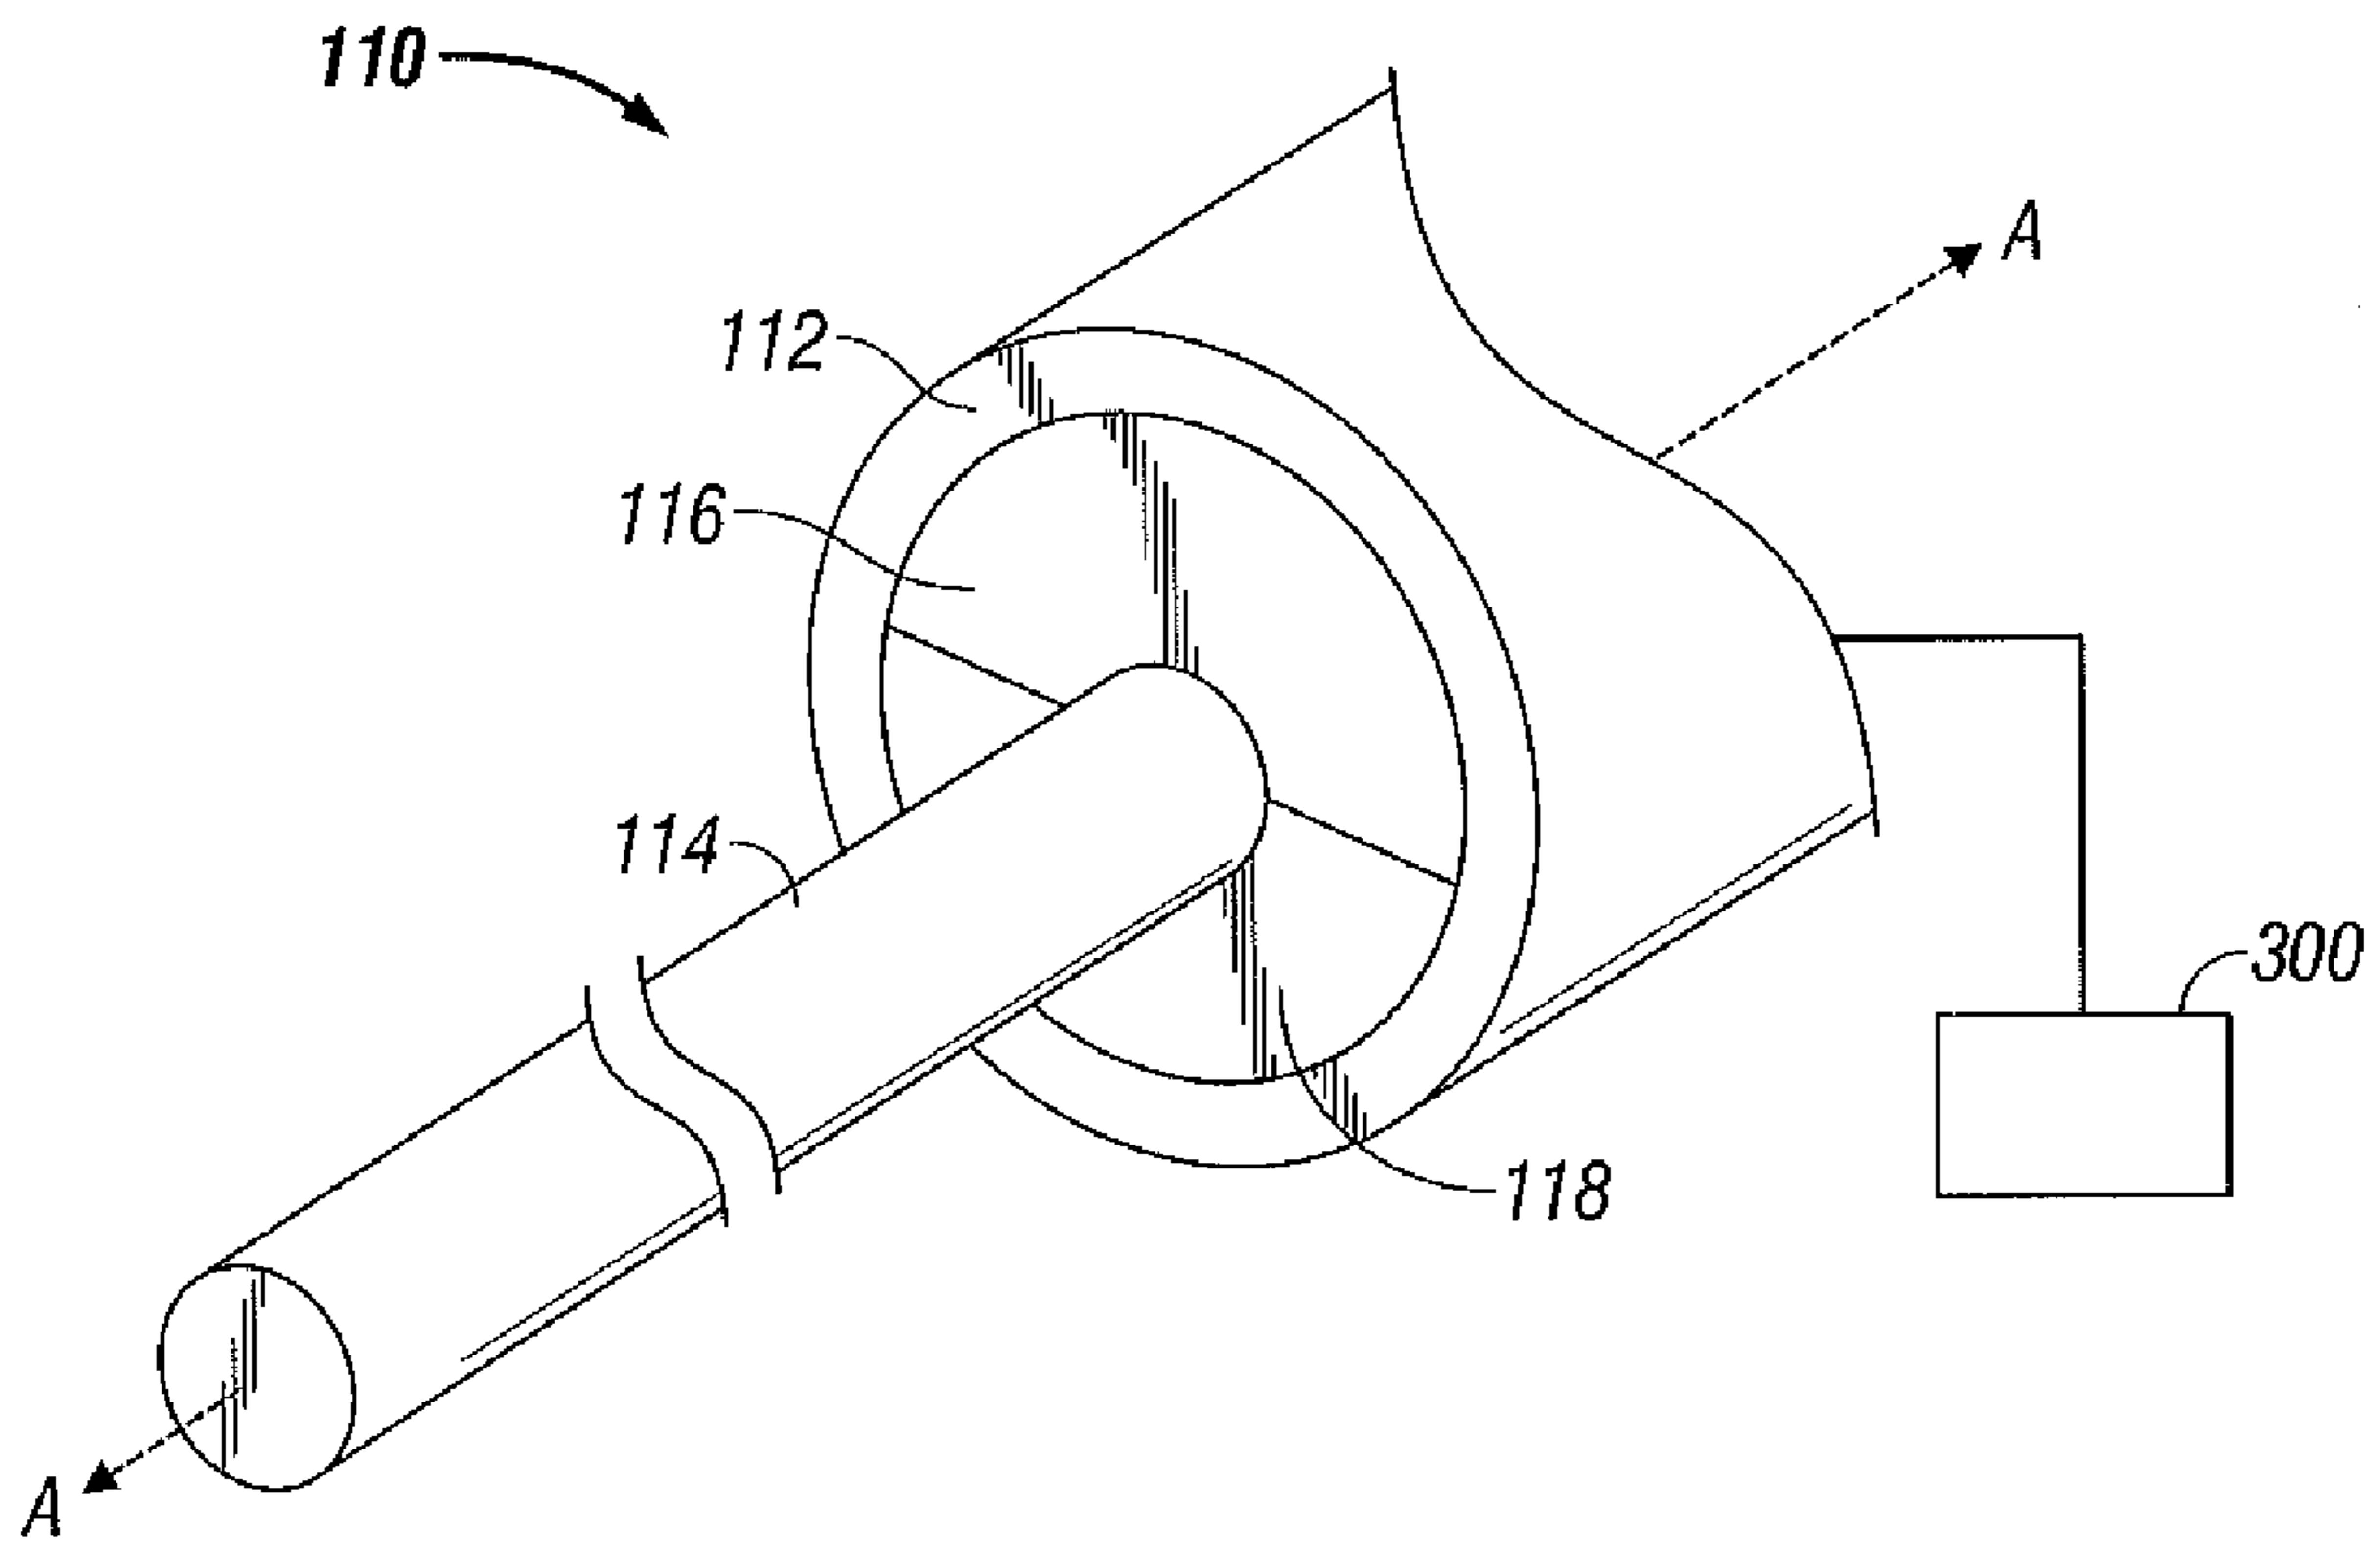


FIG. 2B

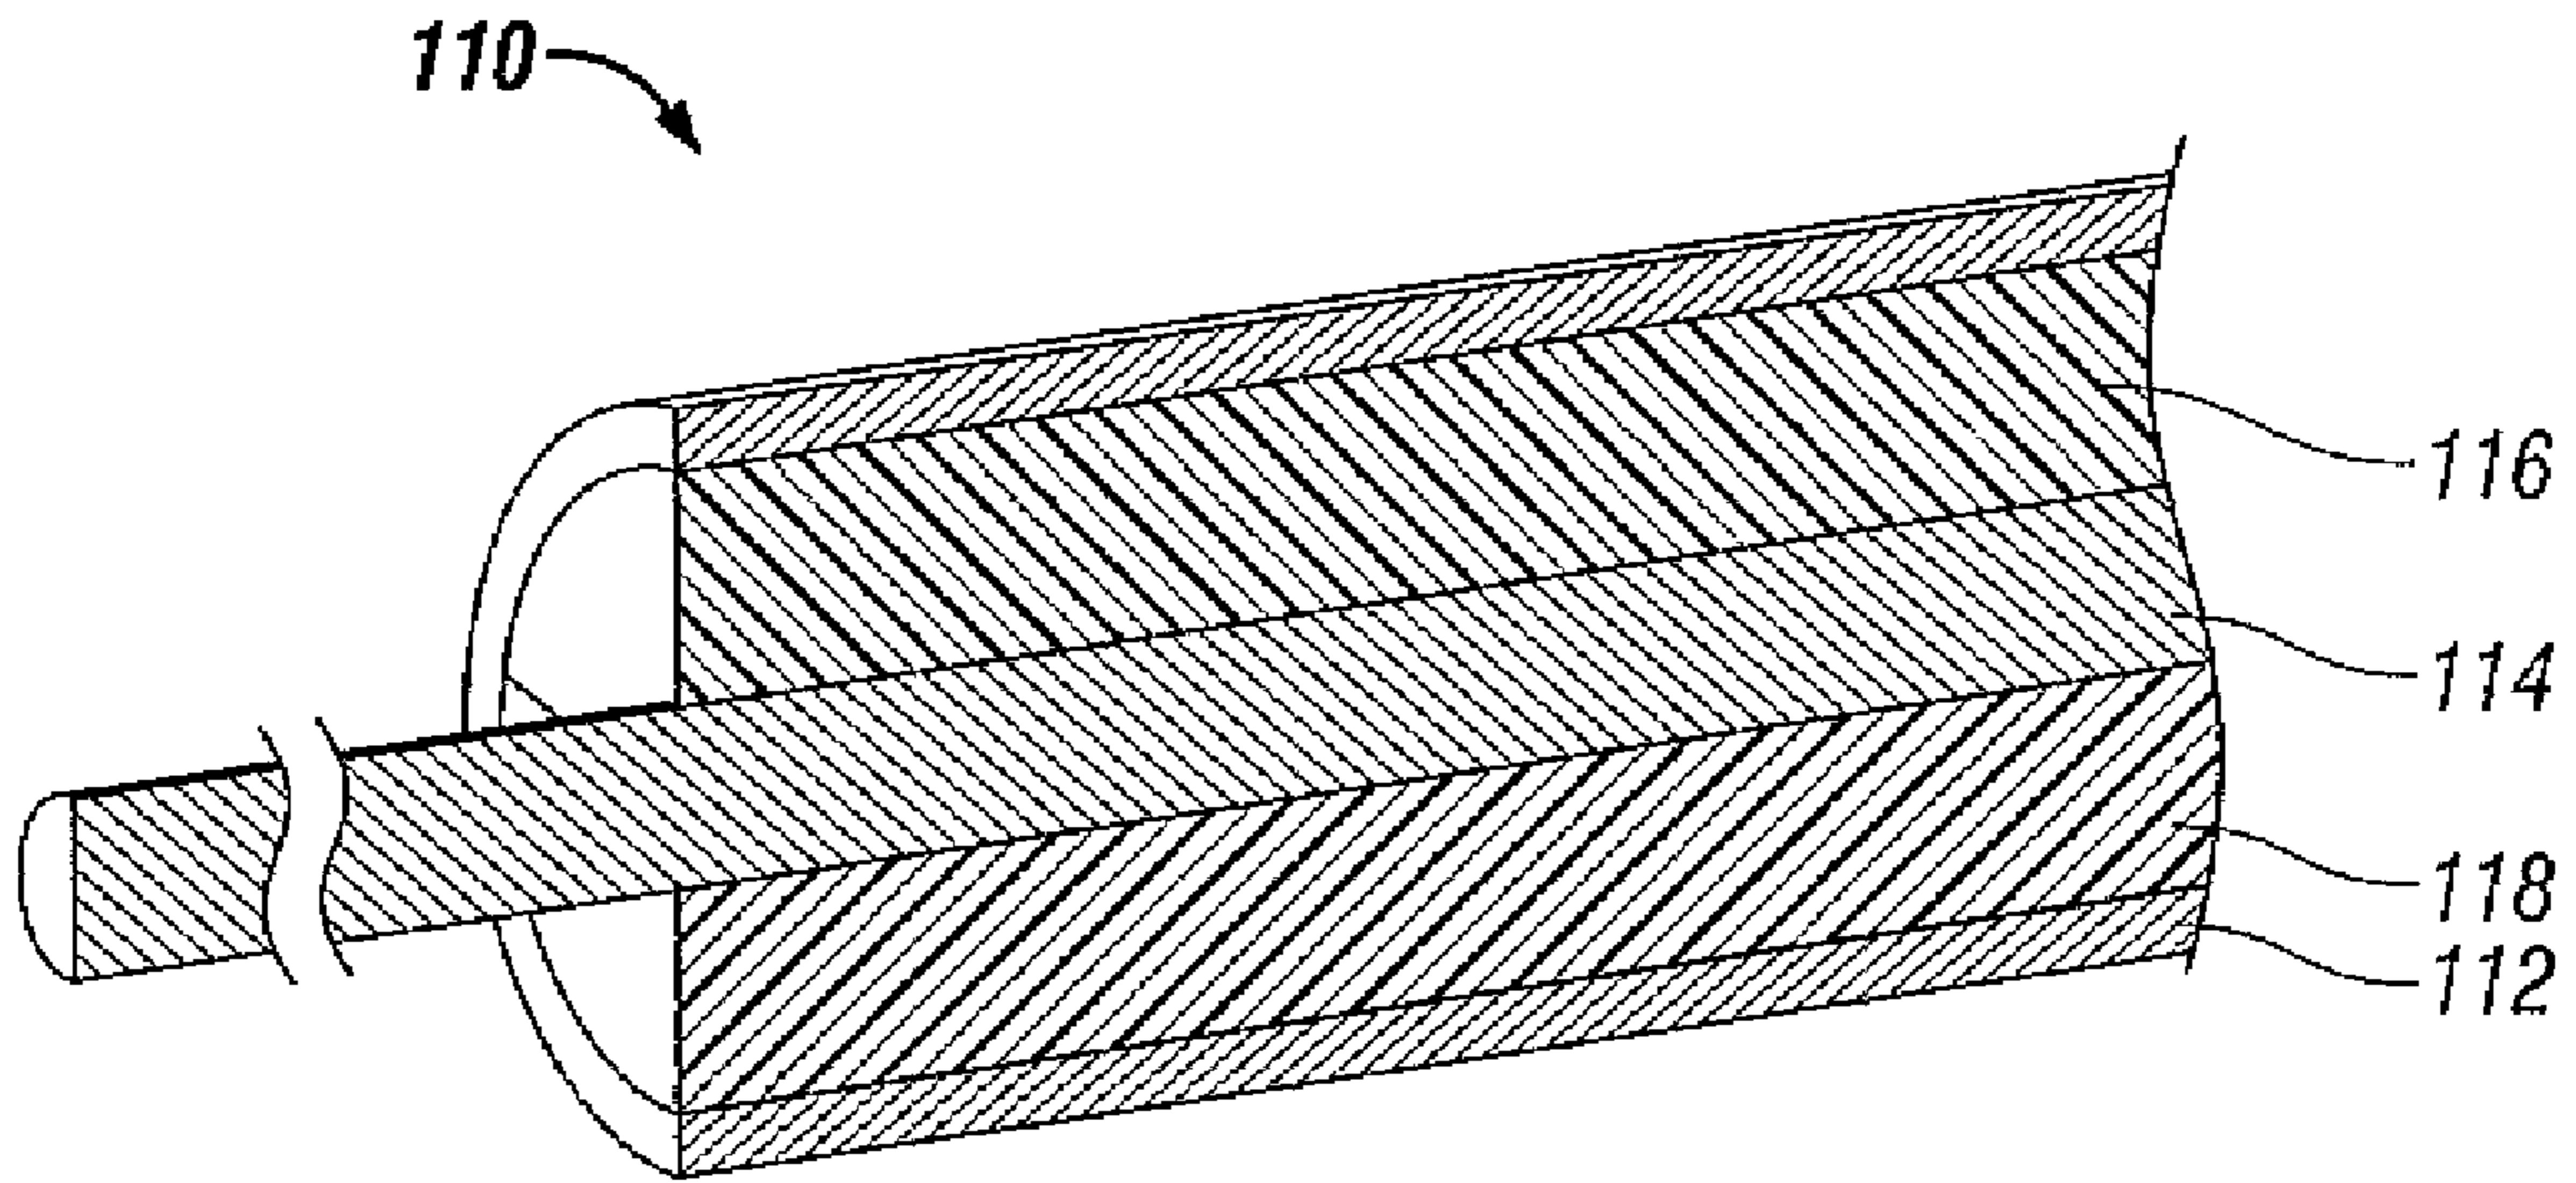


FIG. 2C

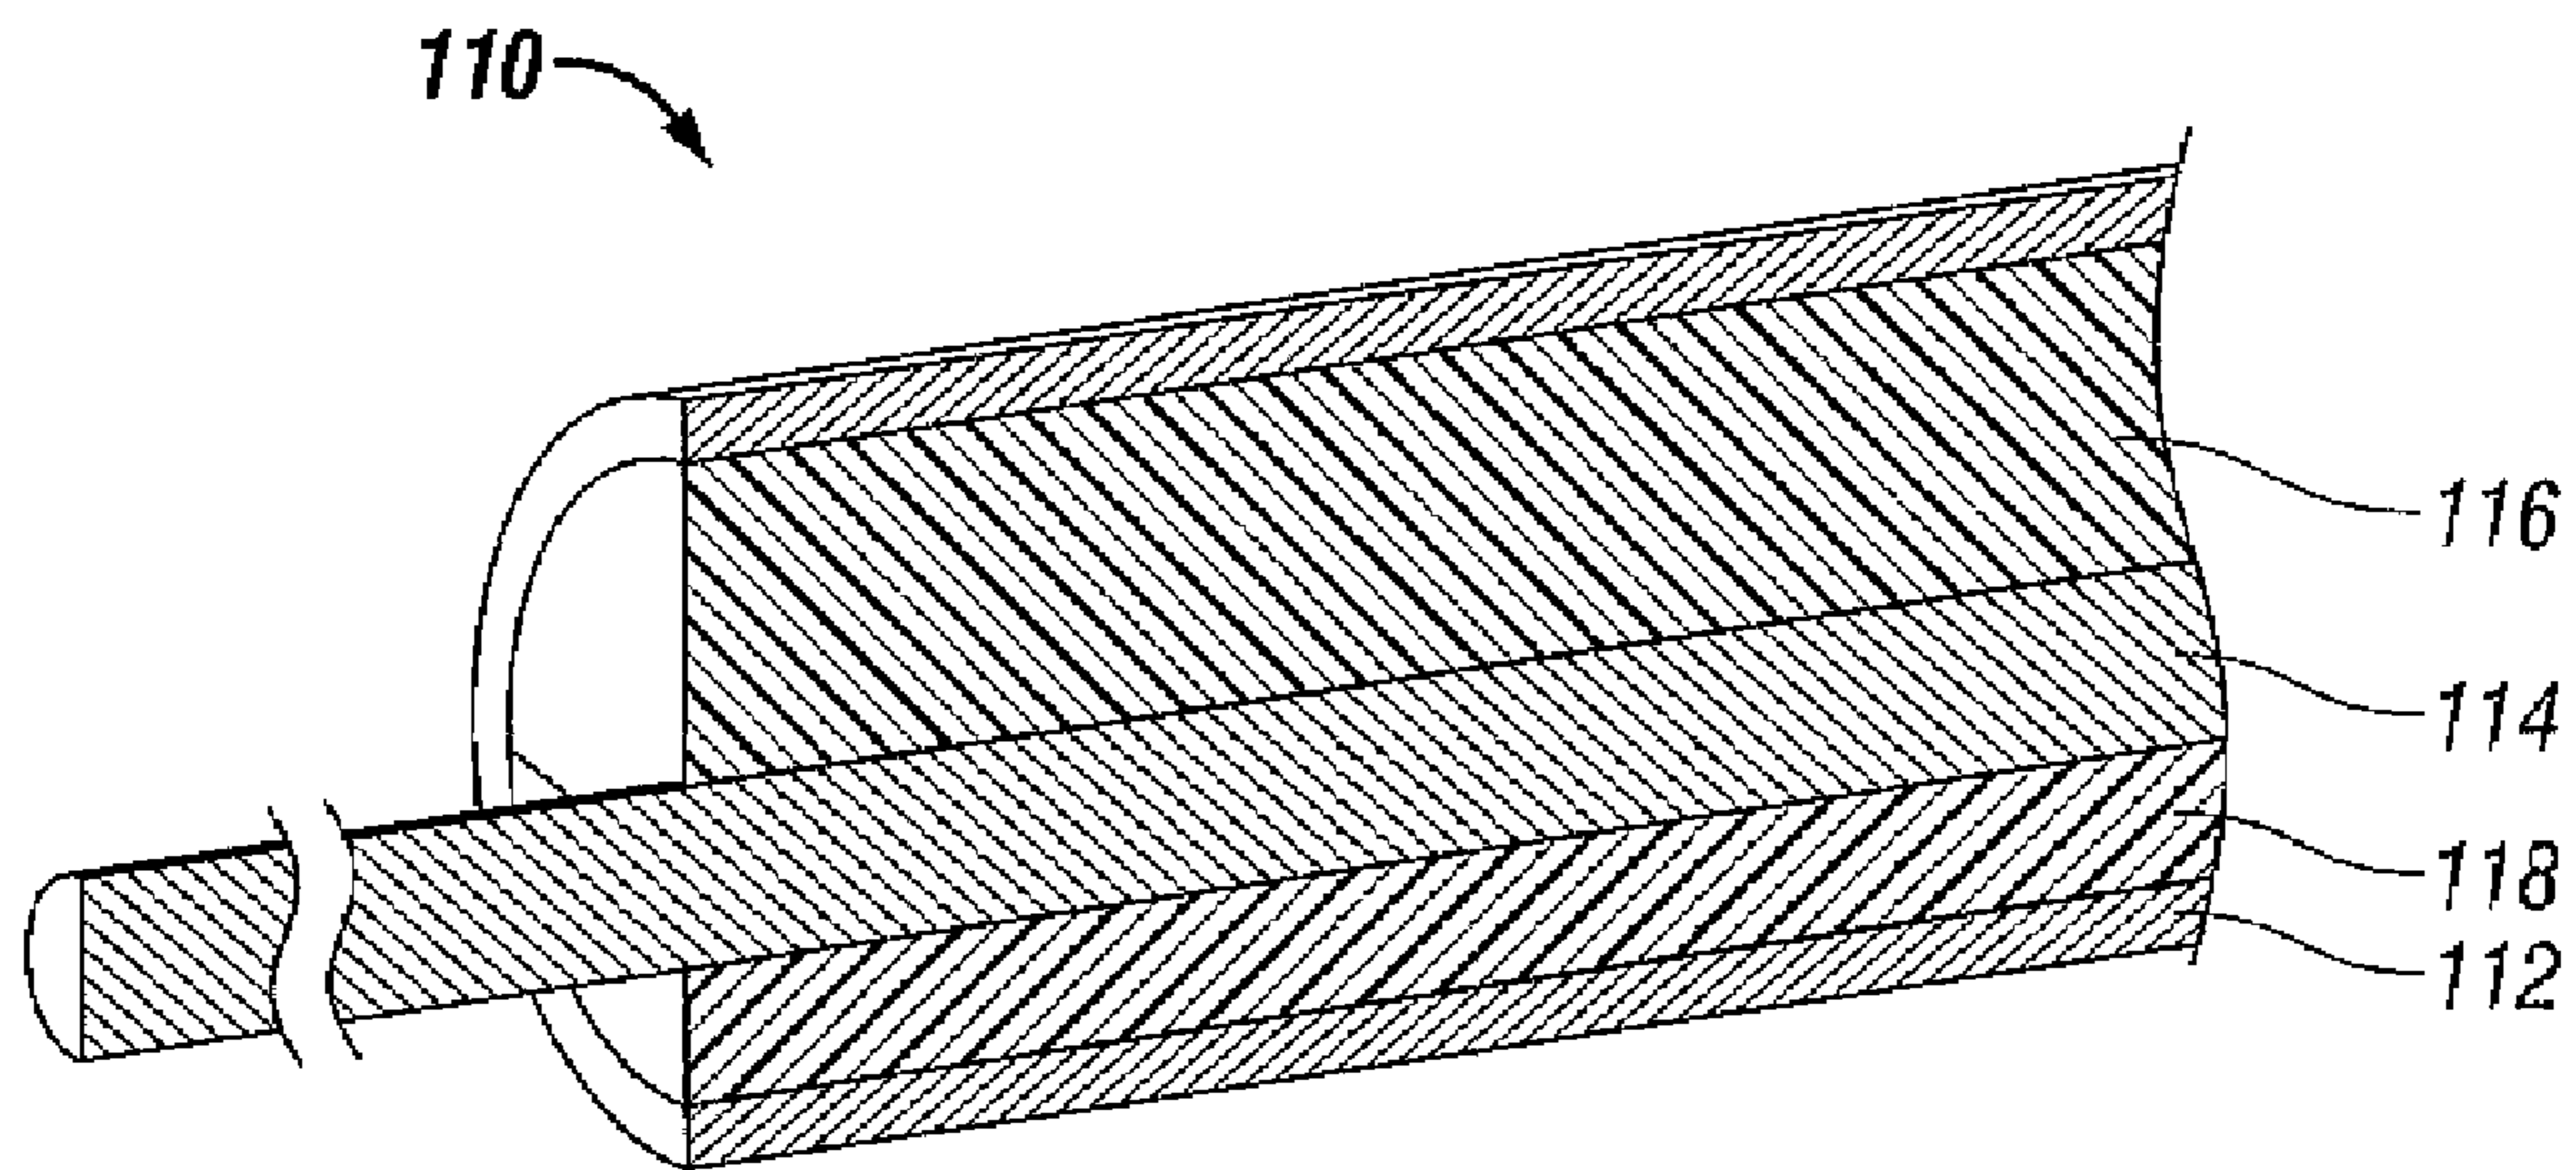


FIG. 2D

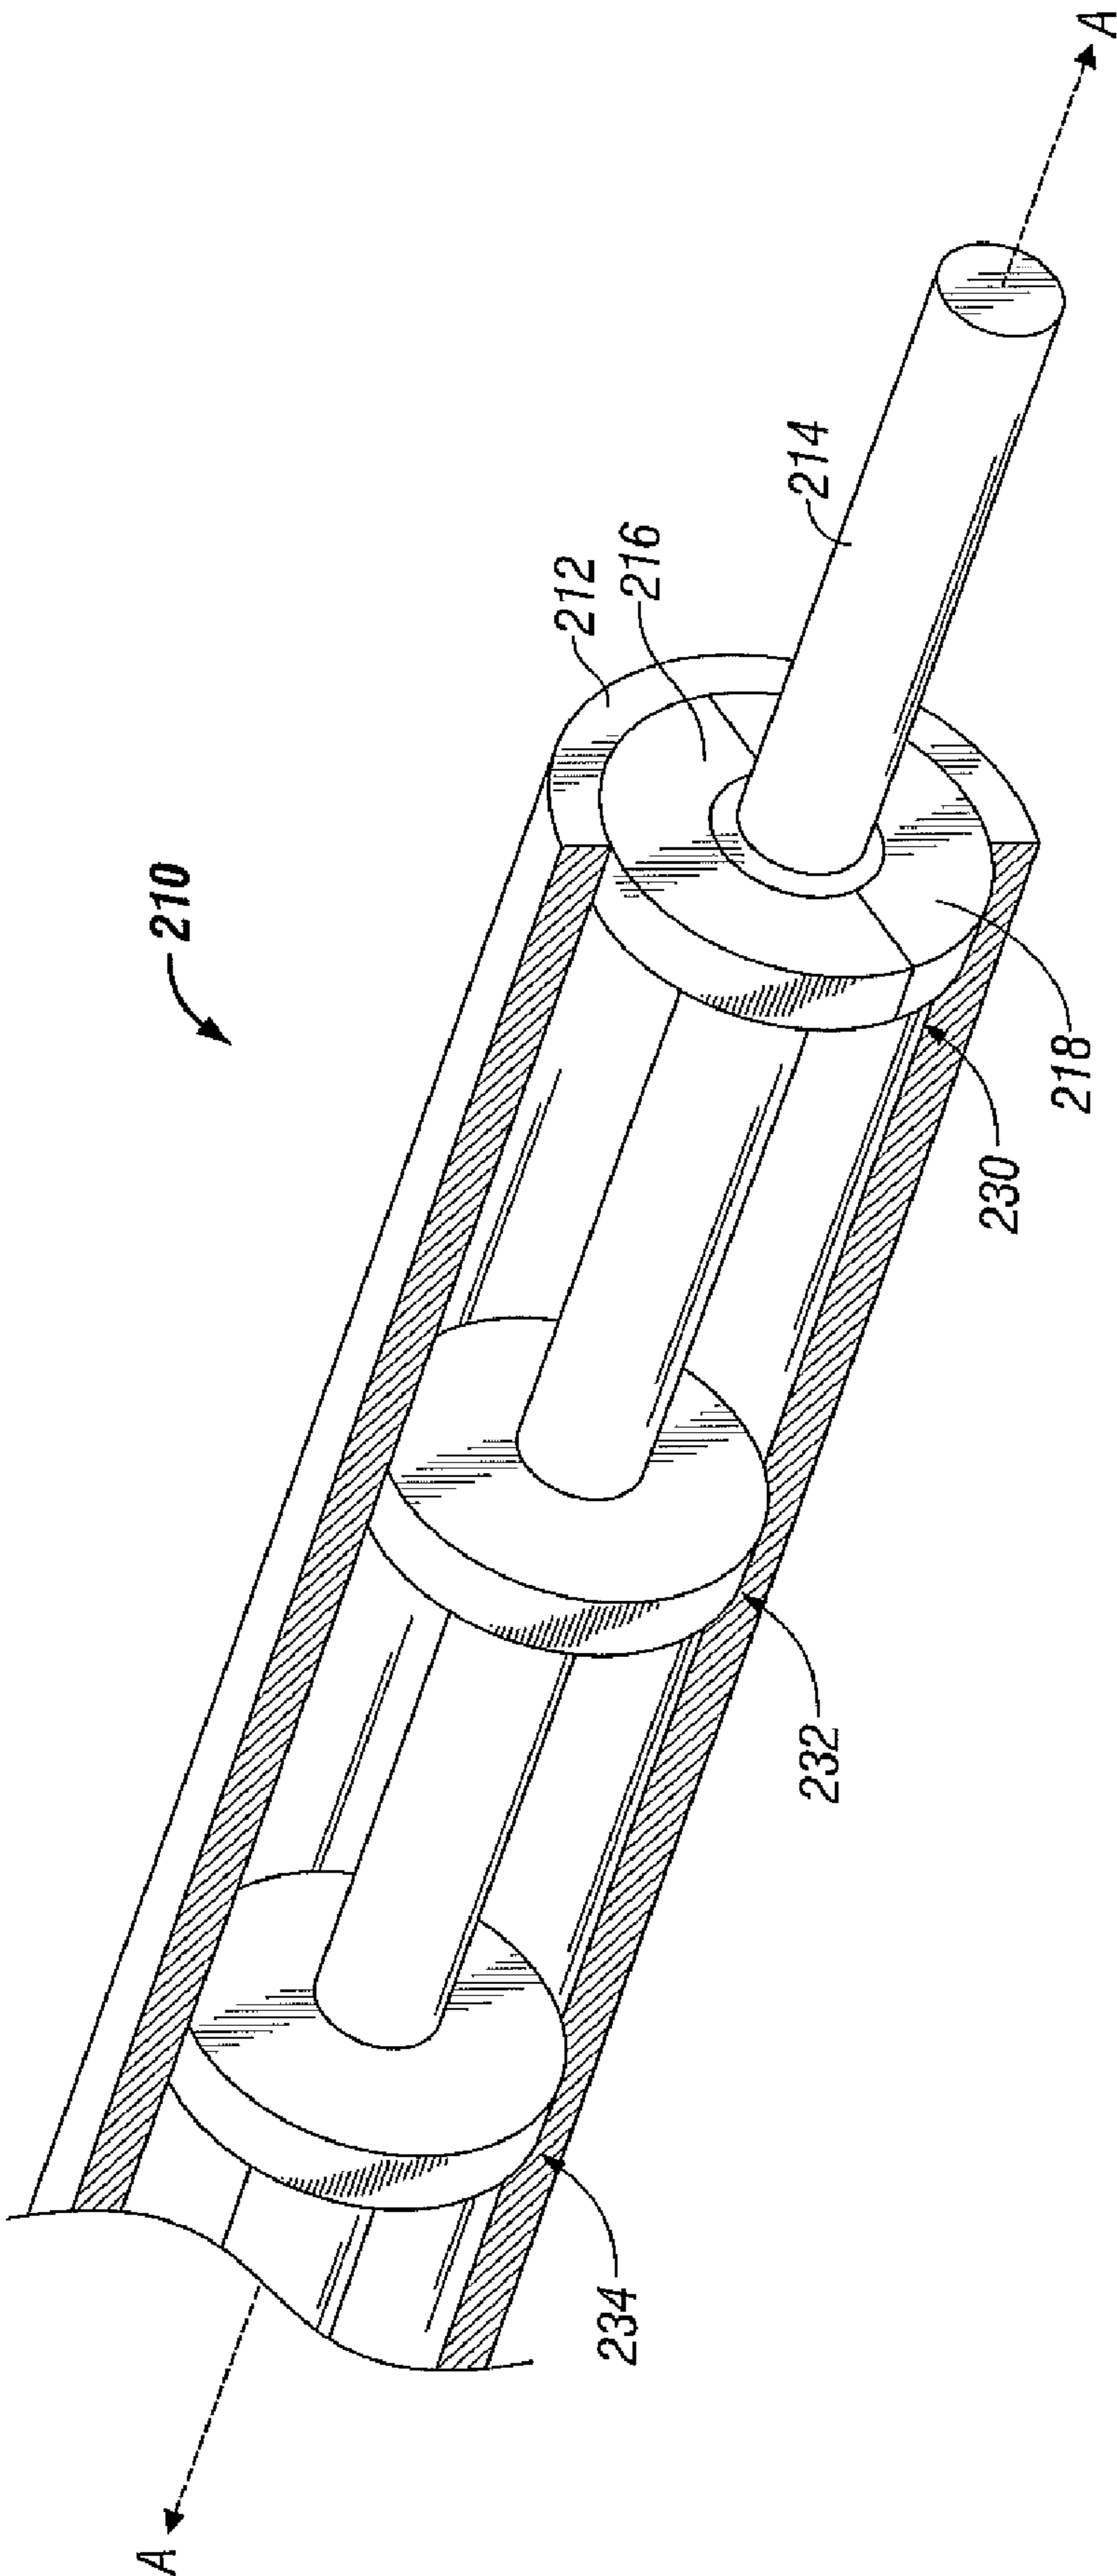


FIG. 3

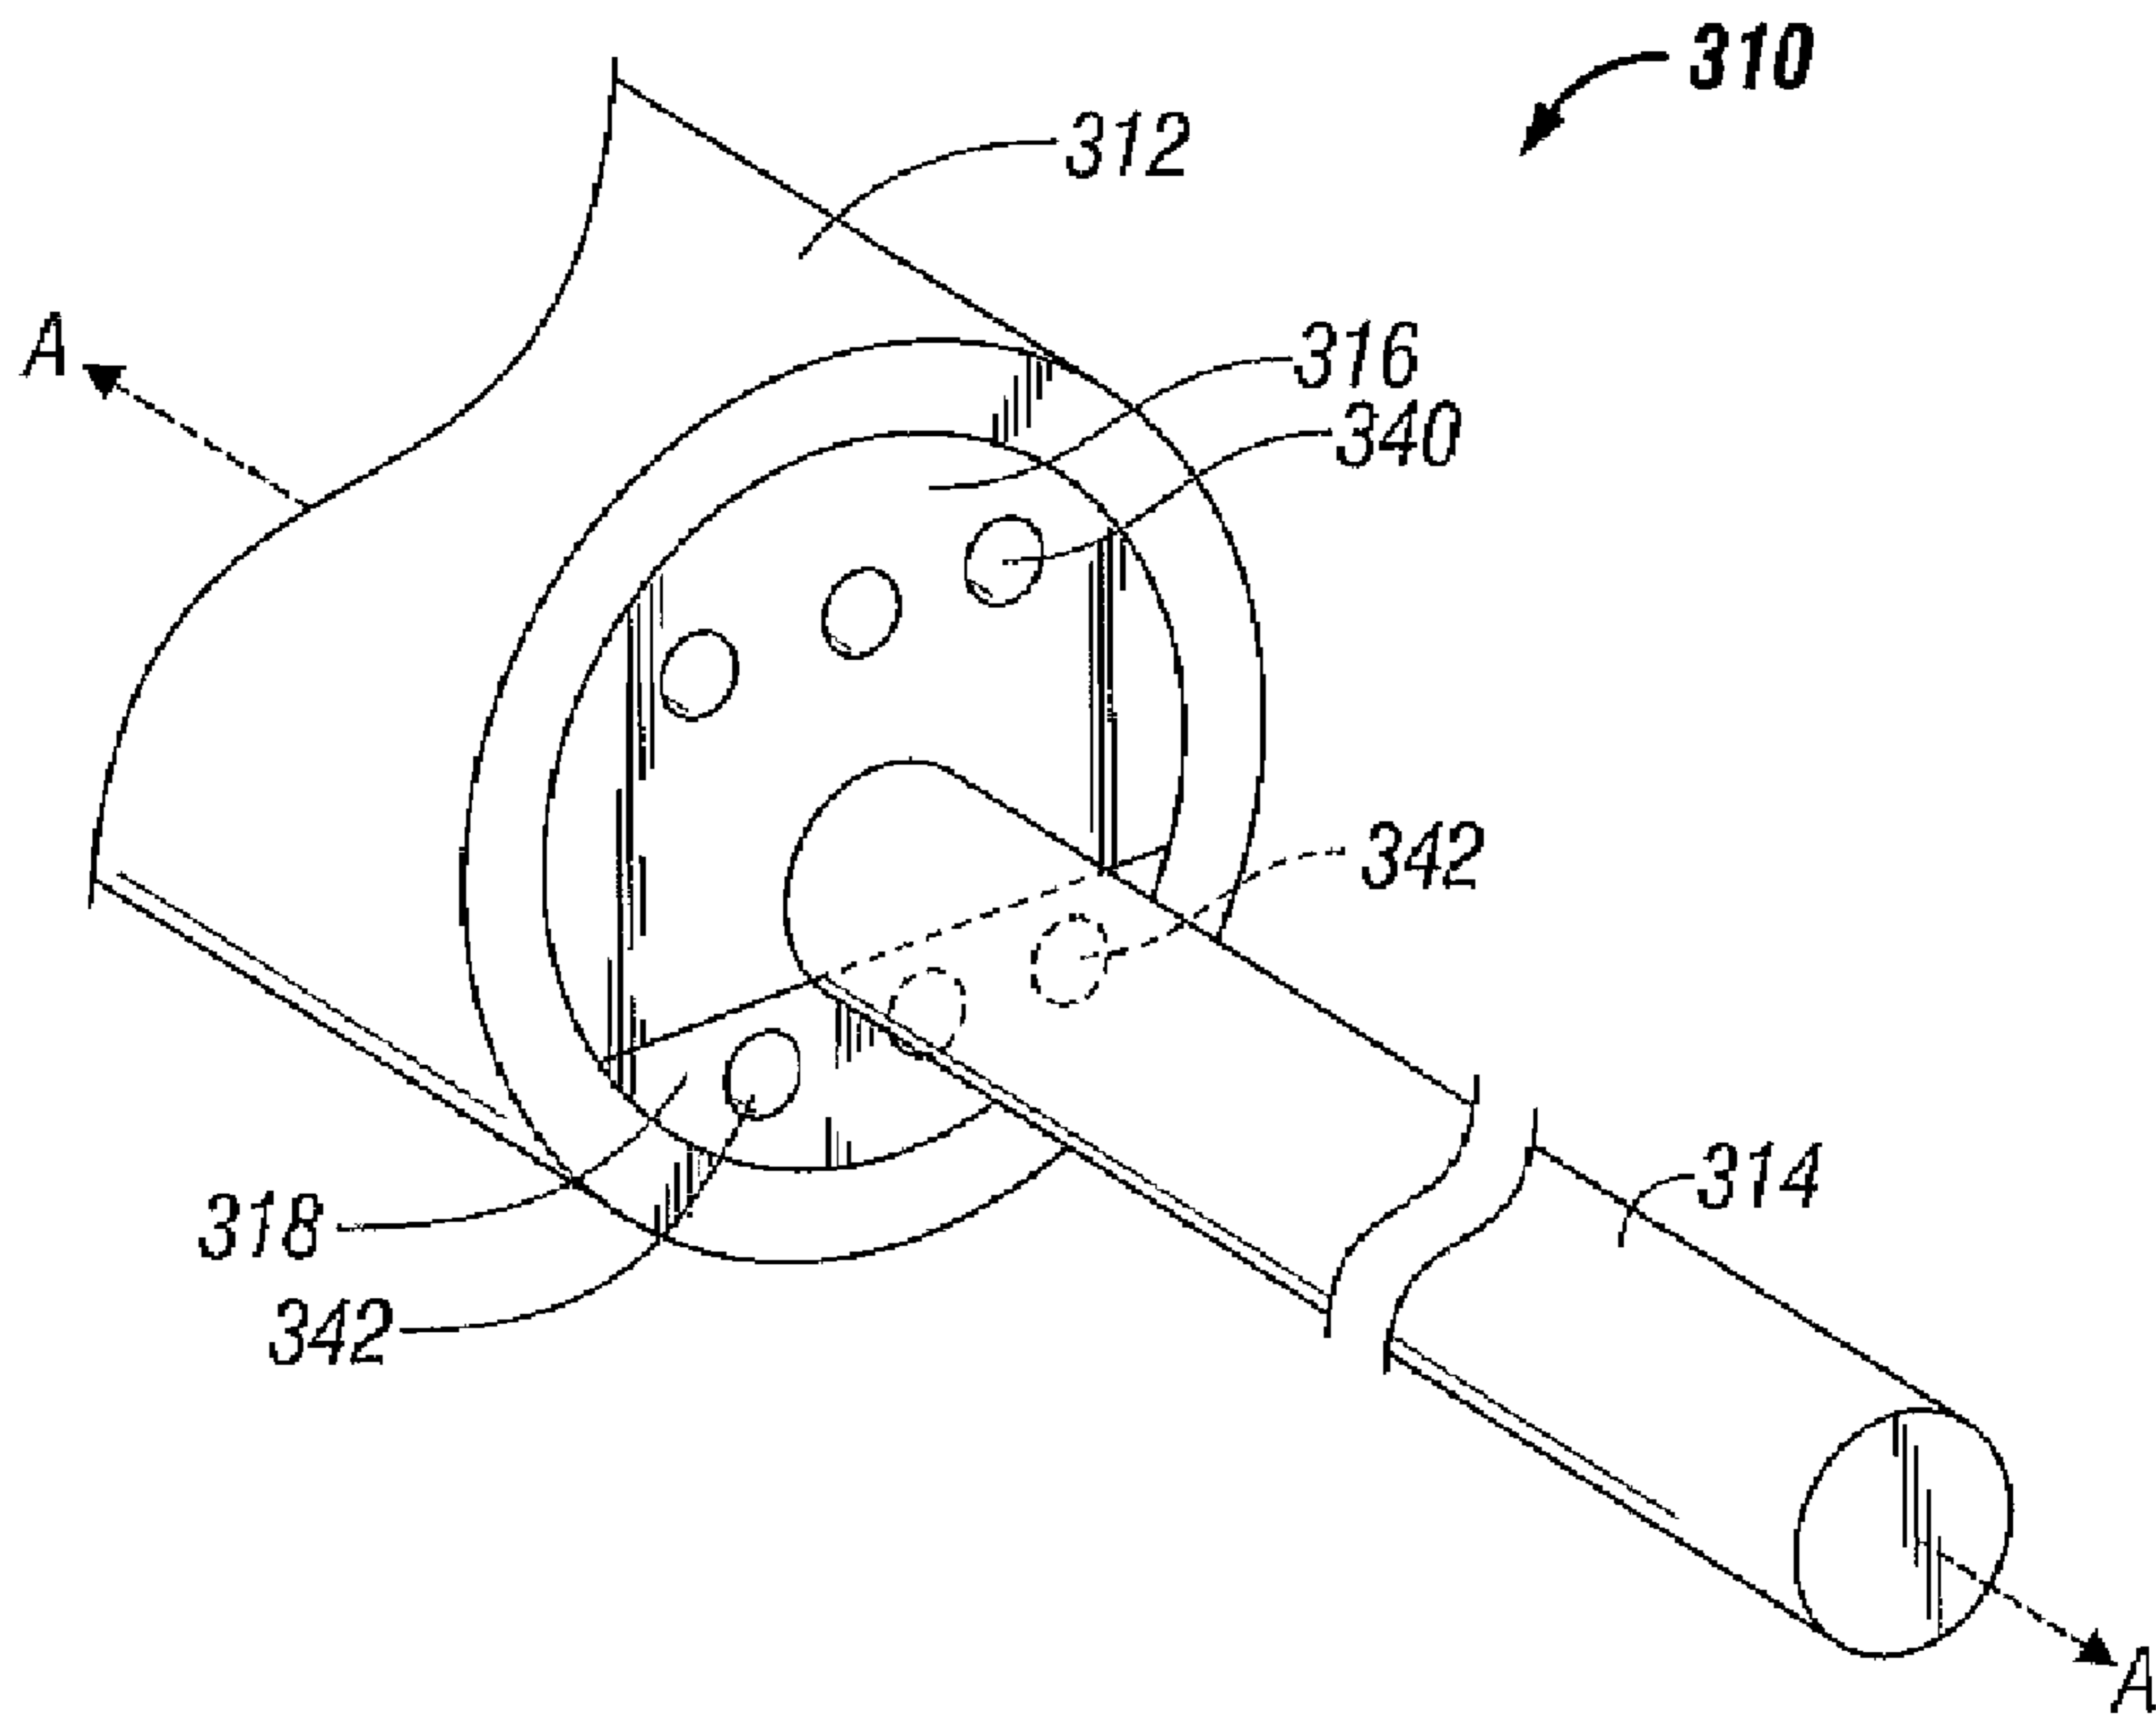


FIG. 4A

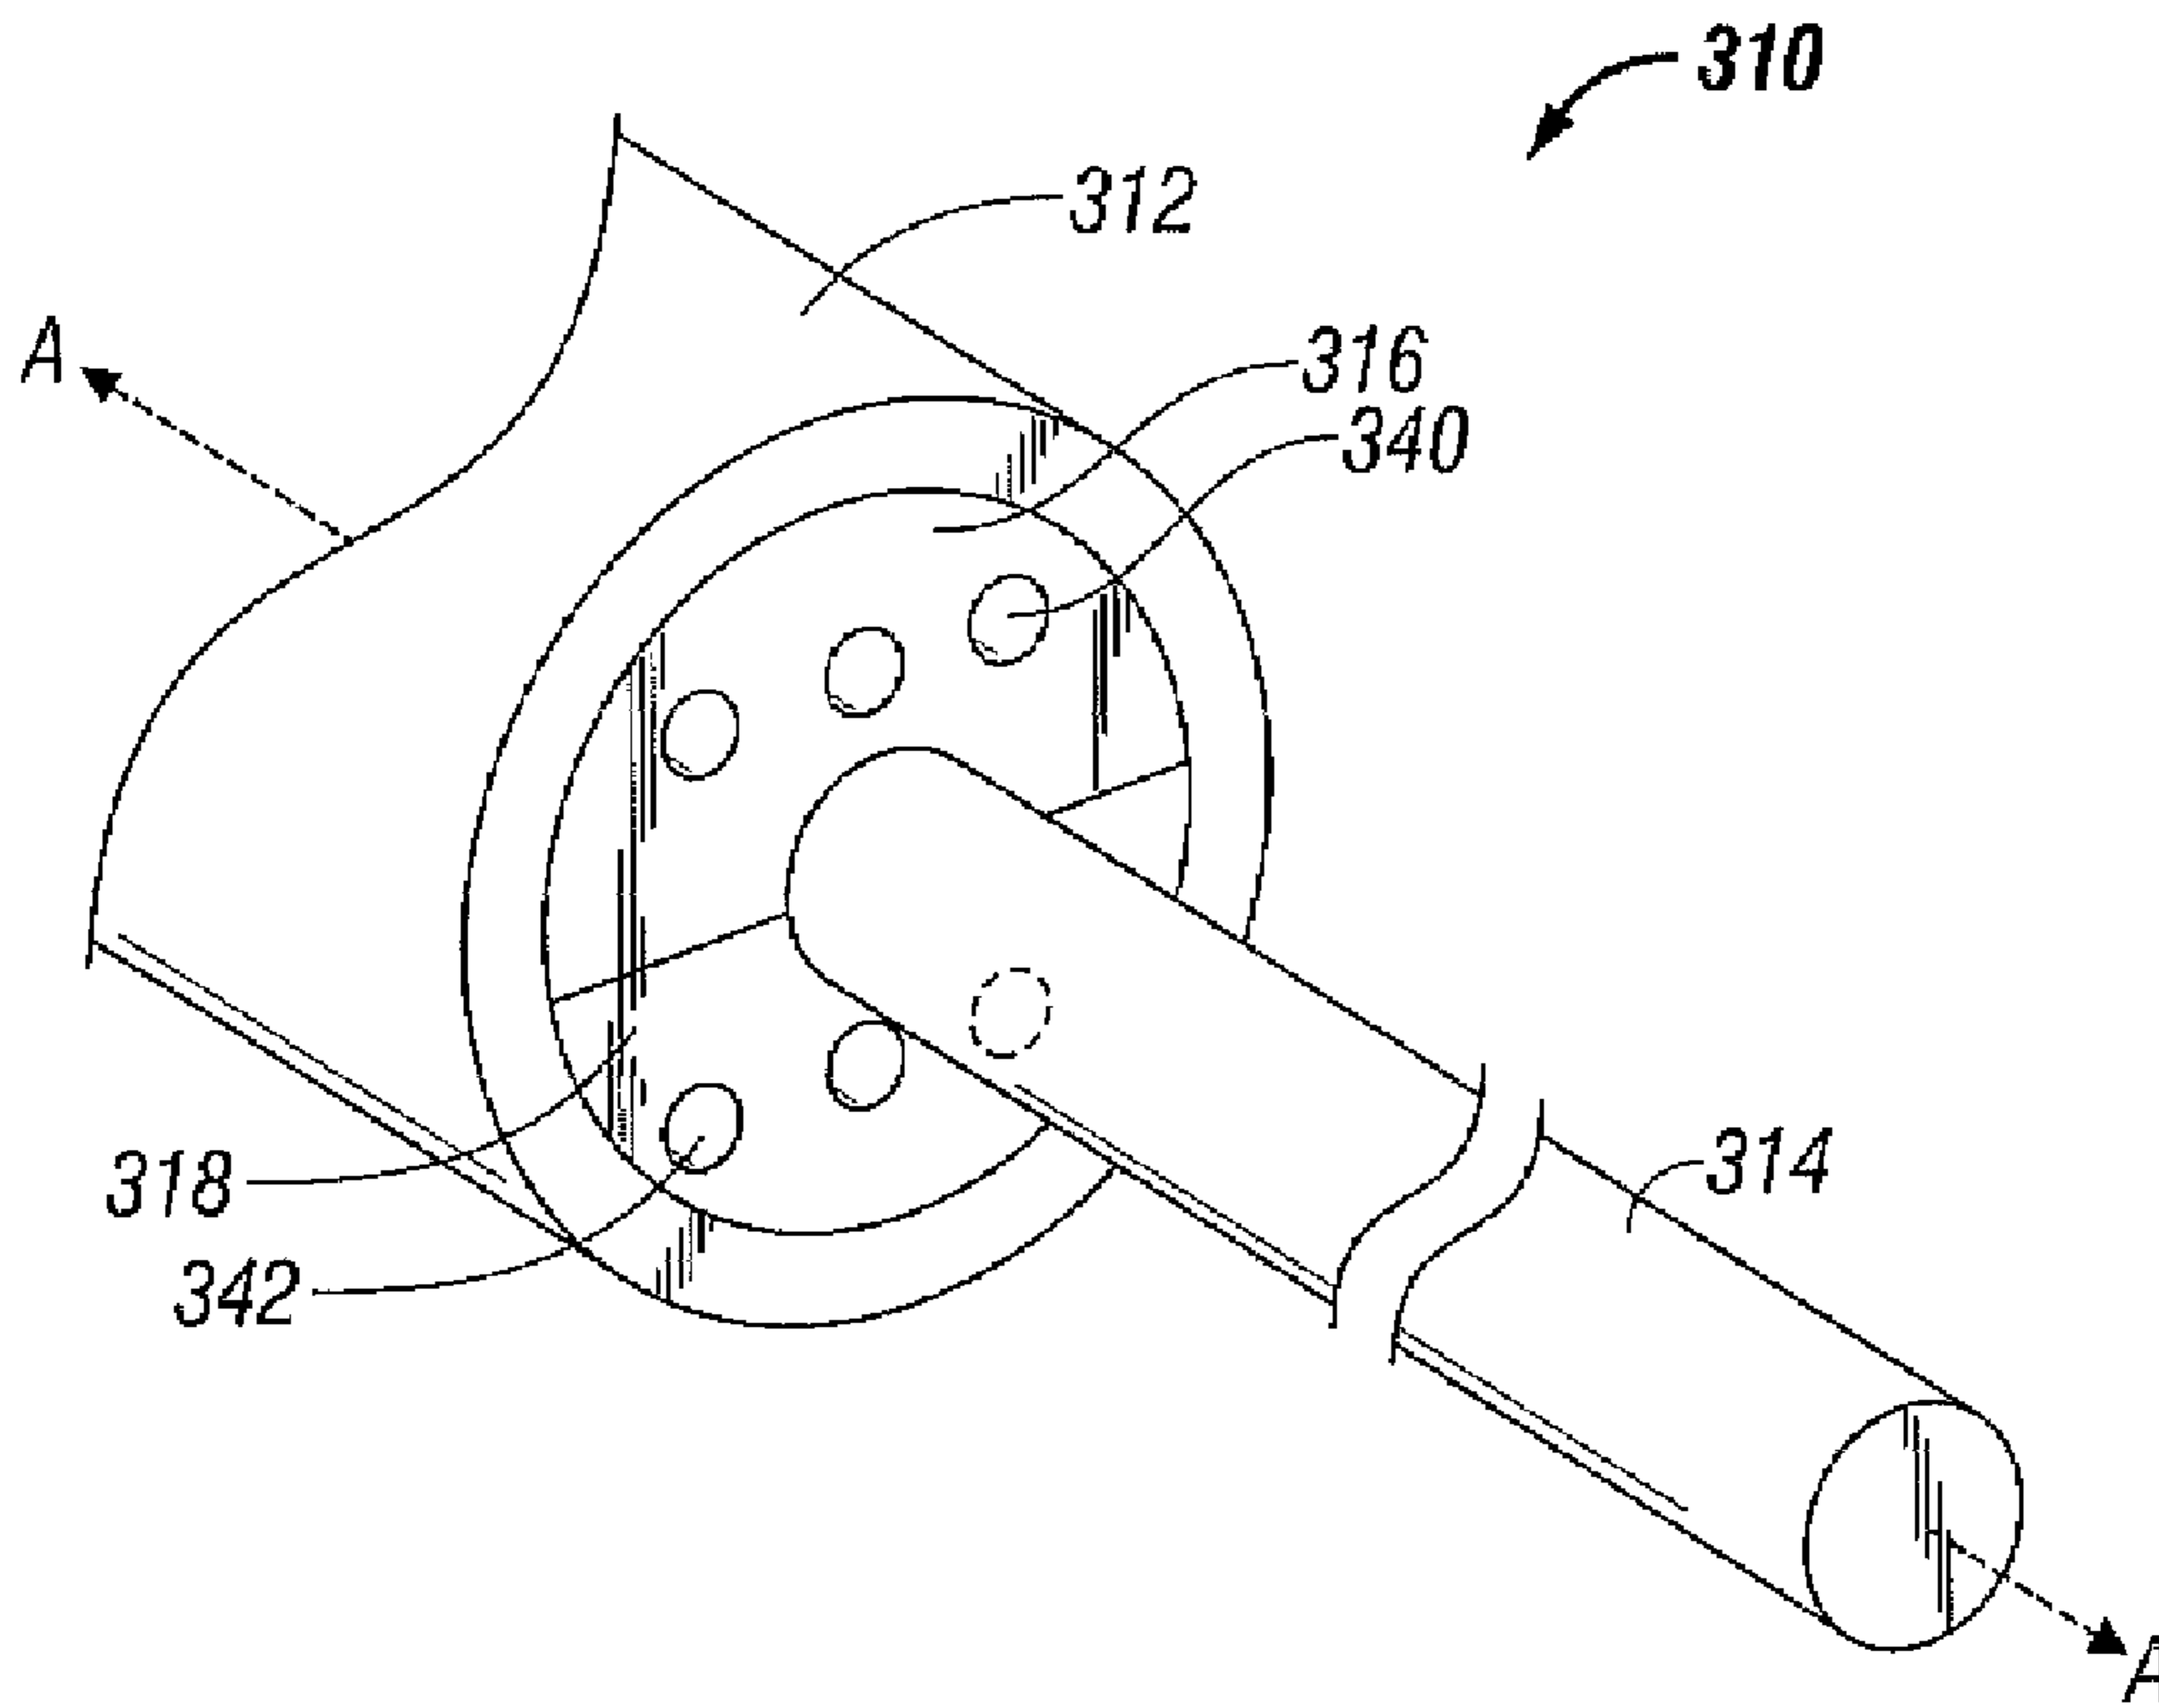


FIG. 4B

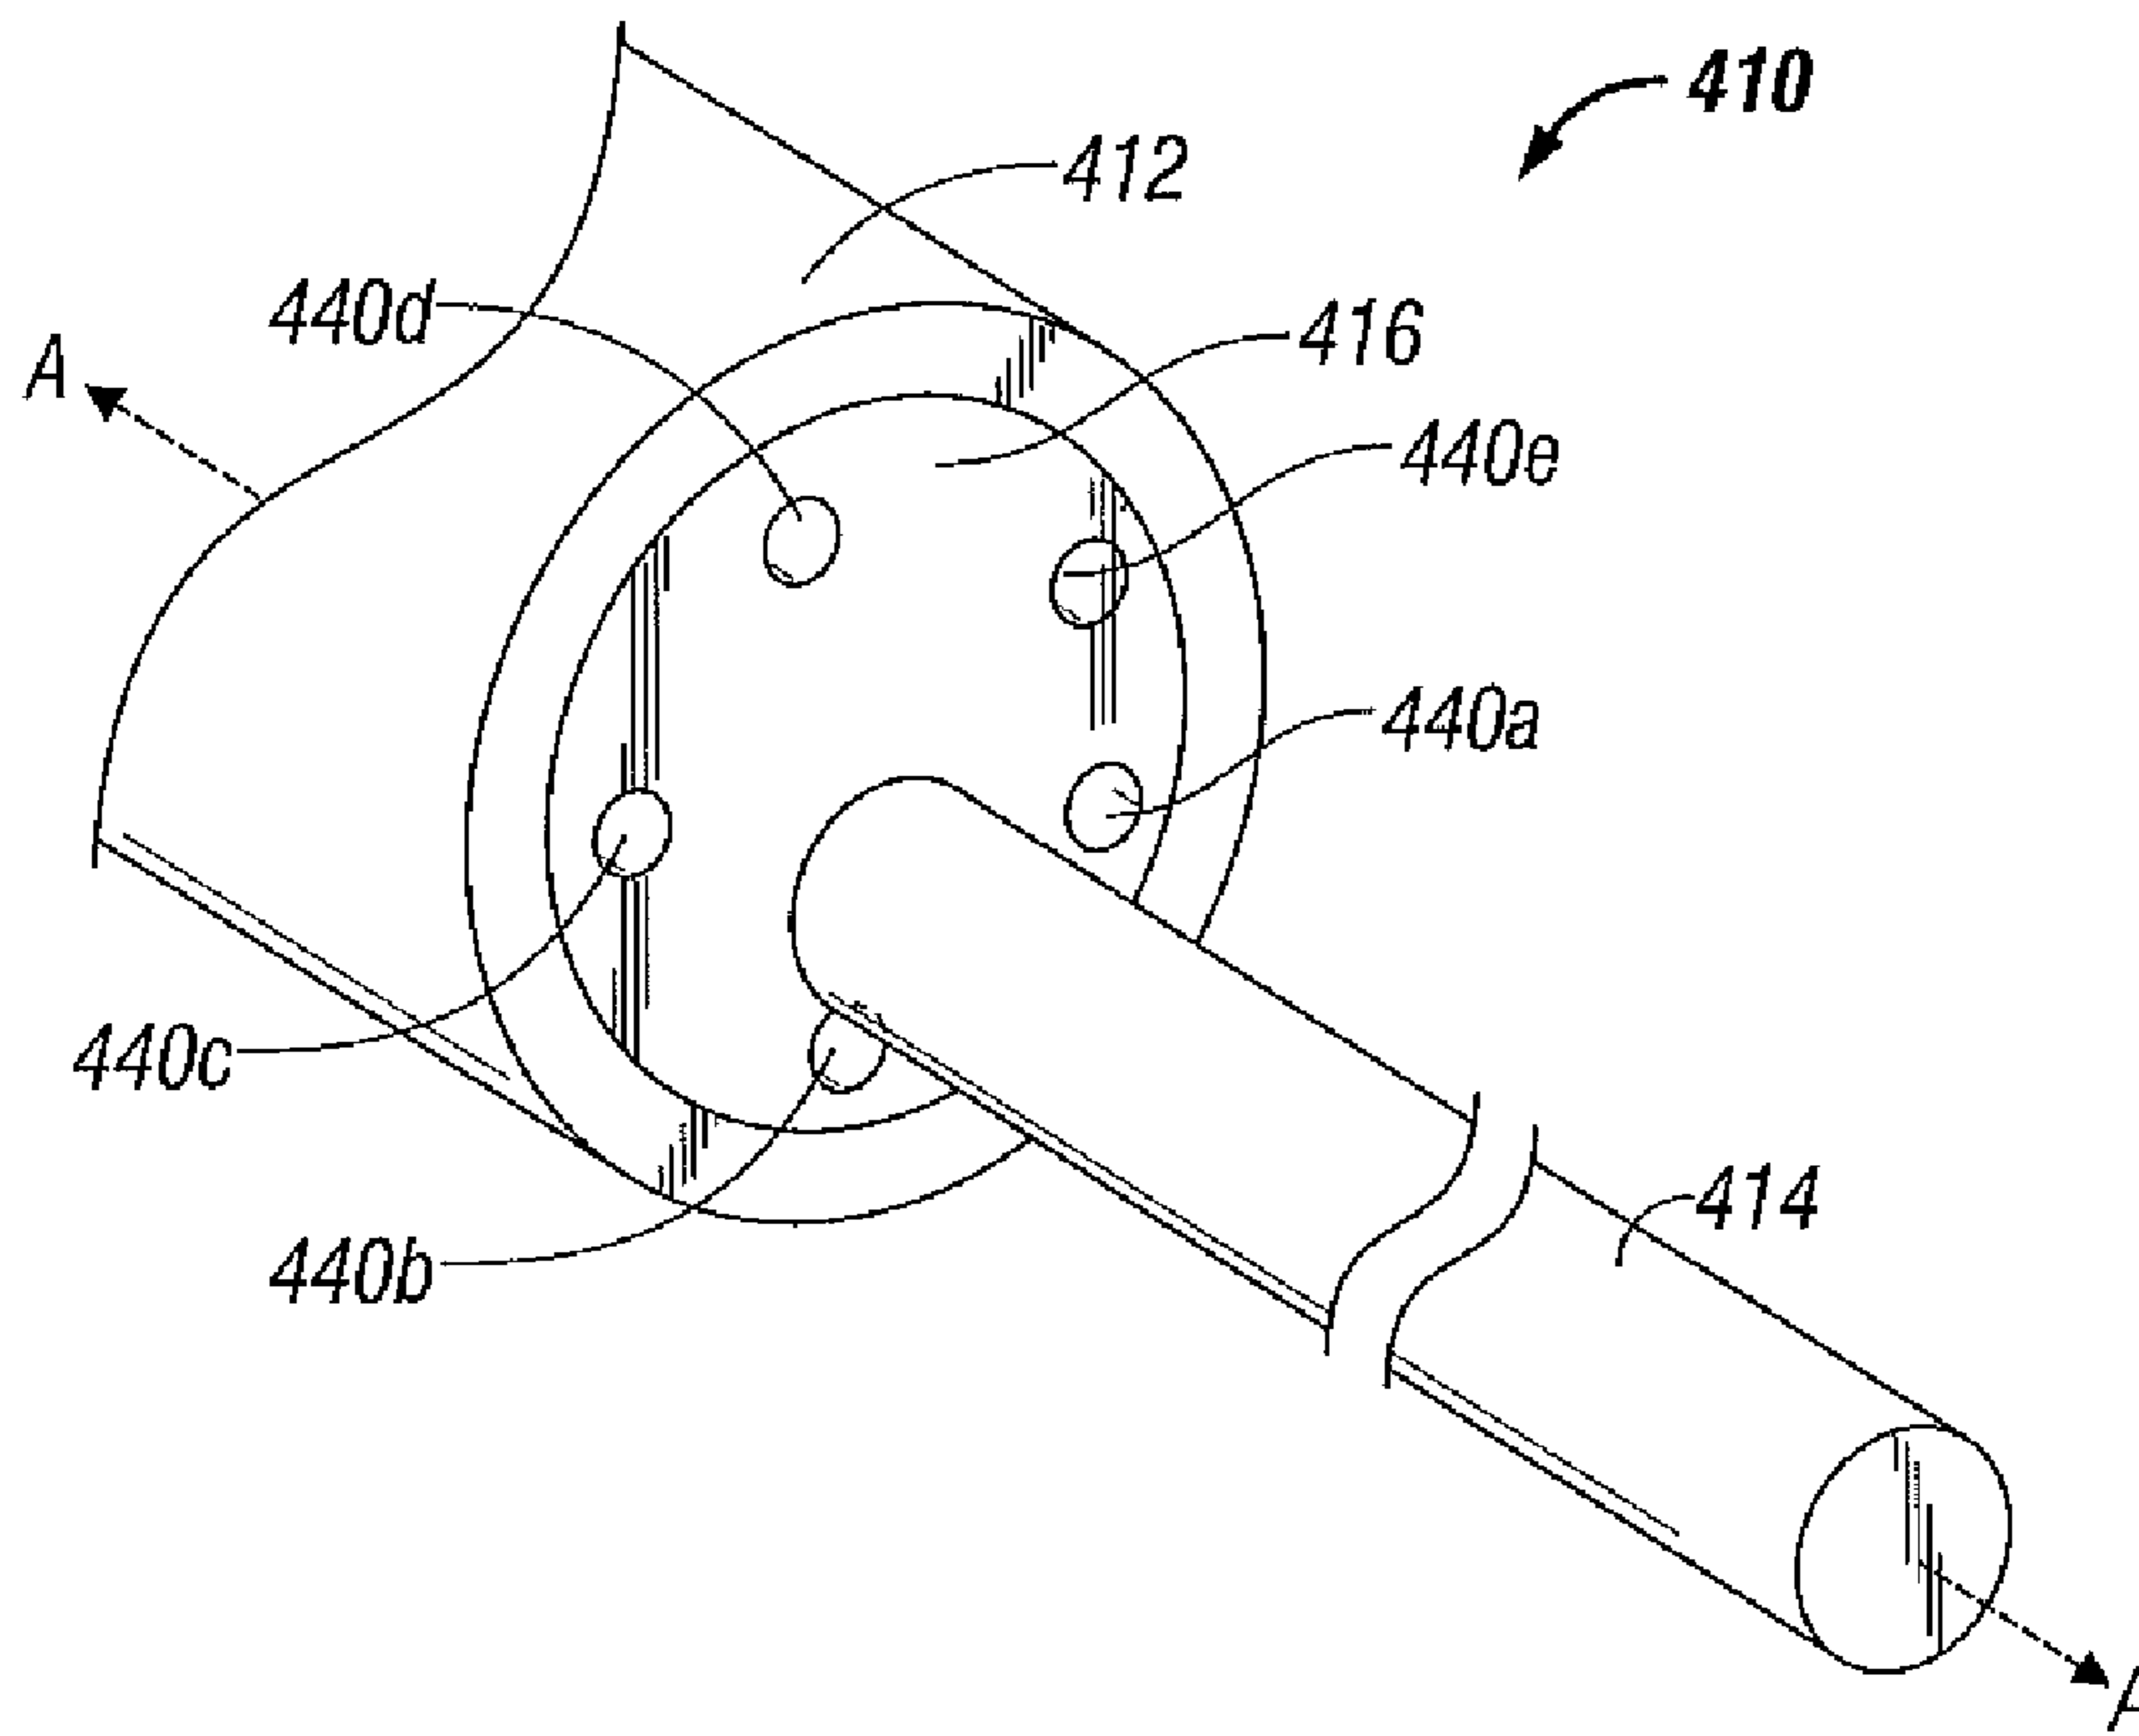


FIG. 5A

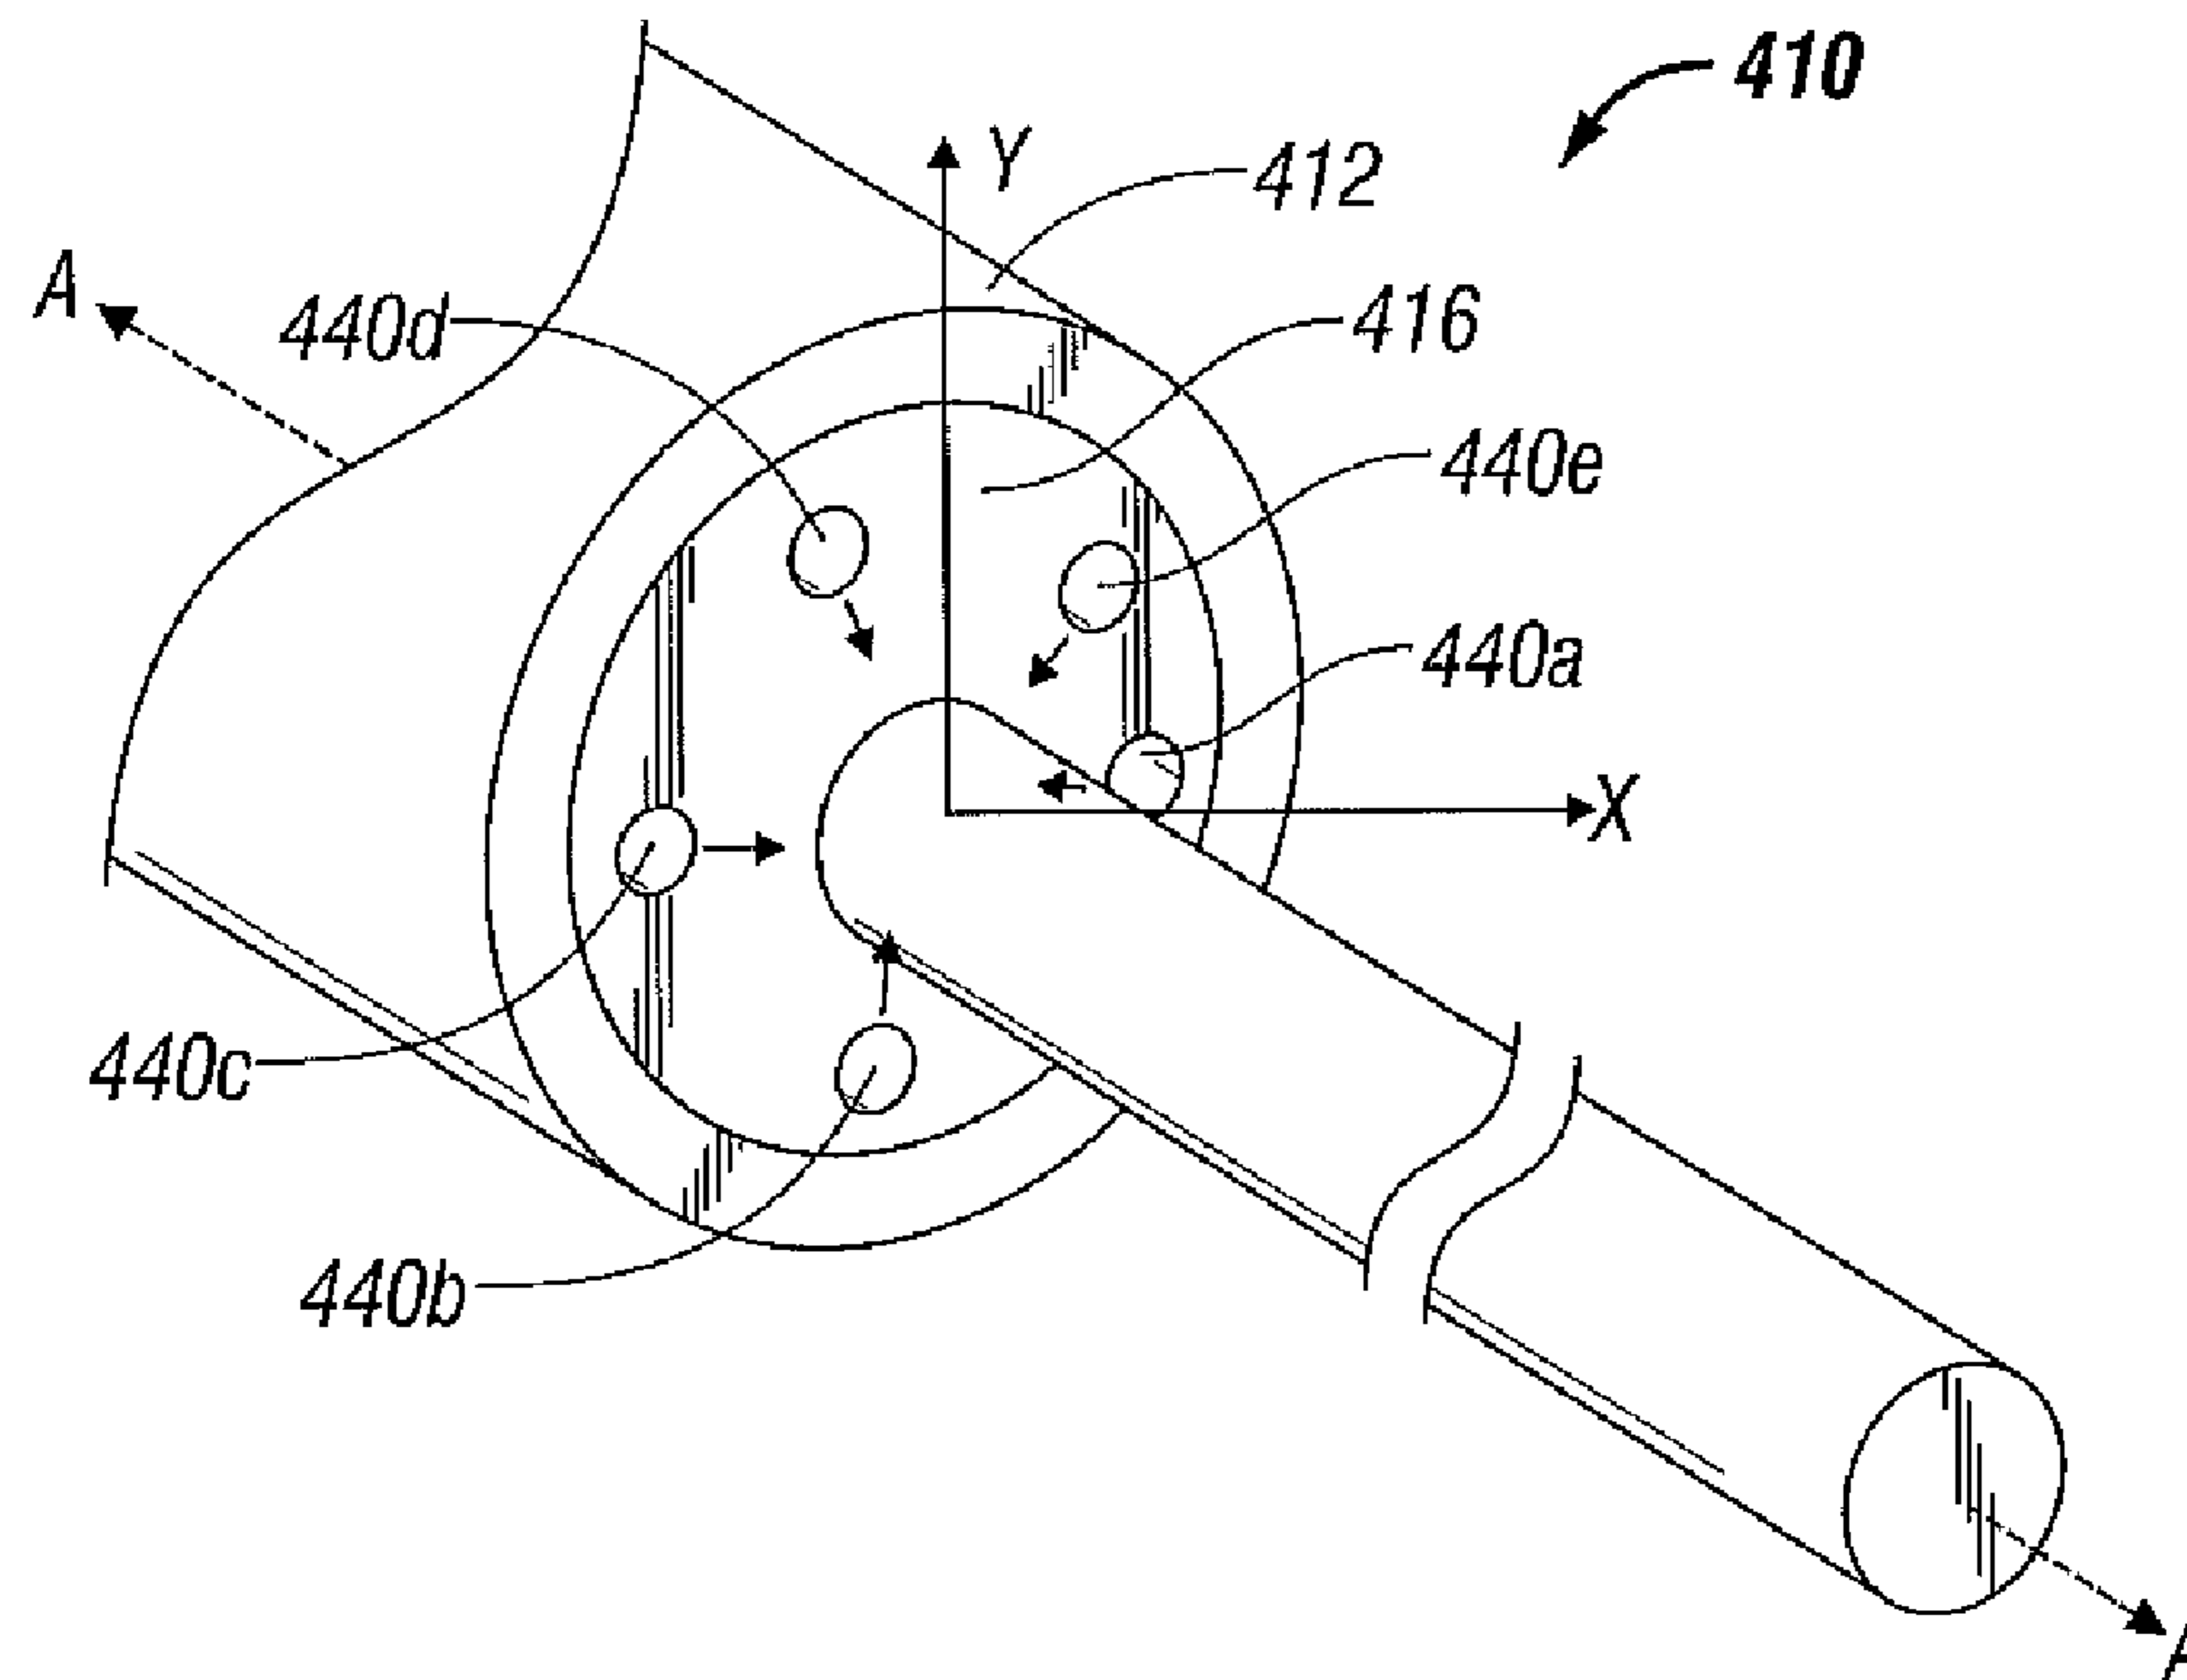


FIG. 5B

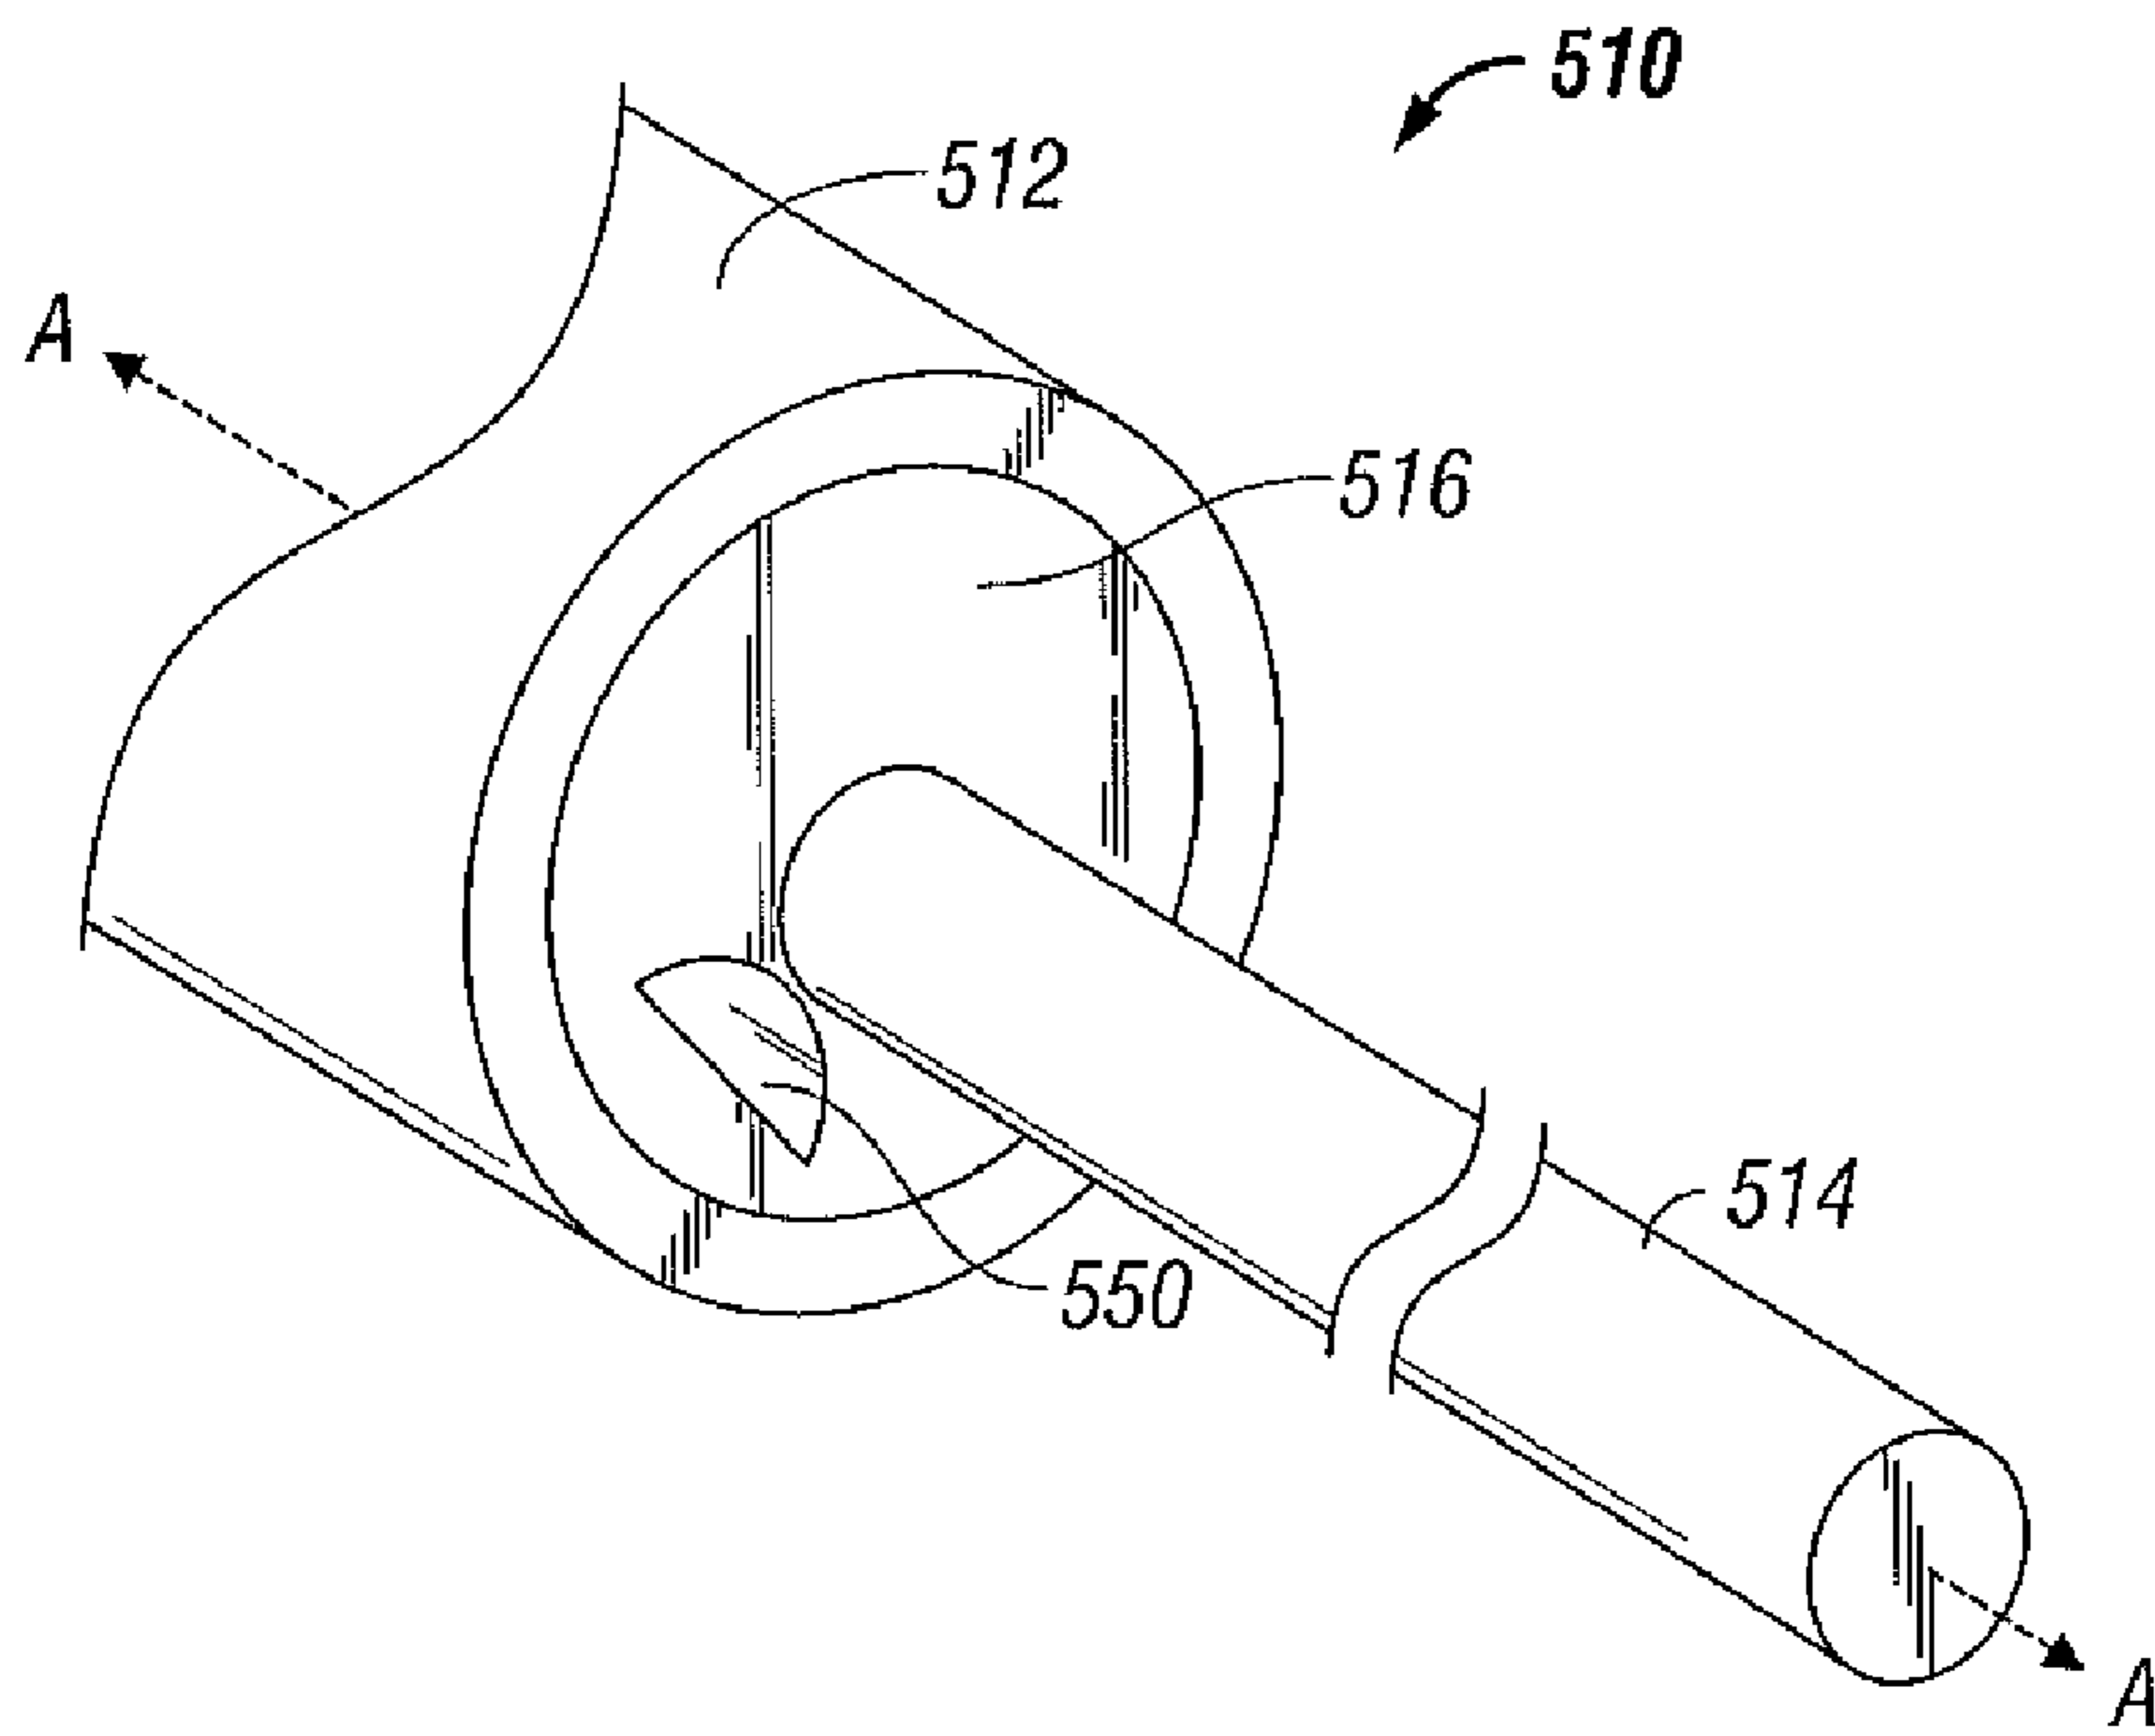


FIG. 6

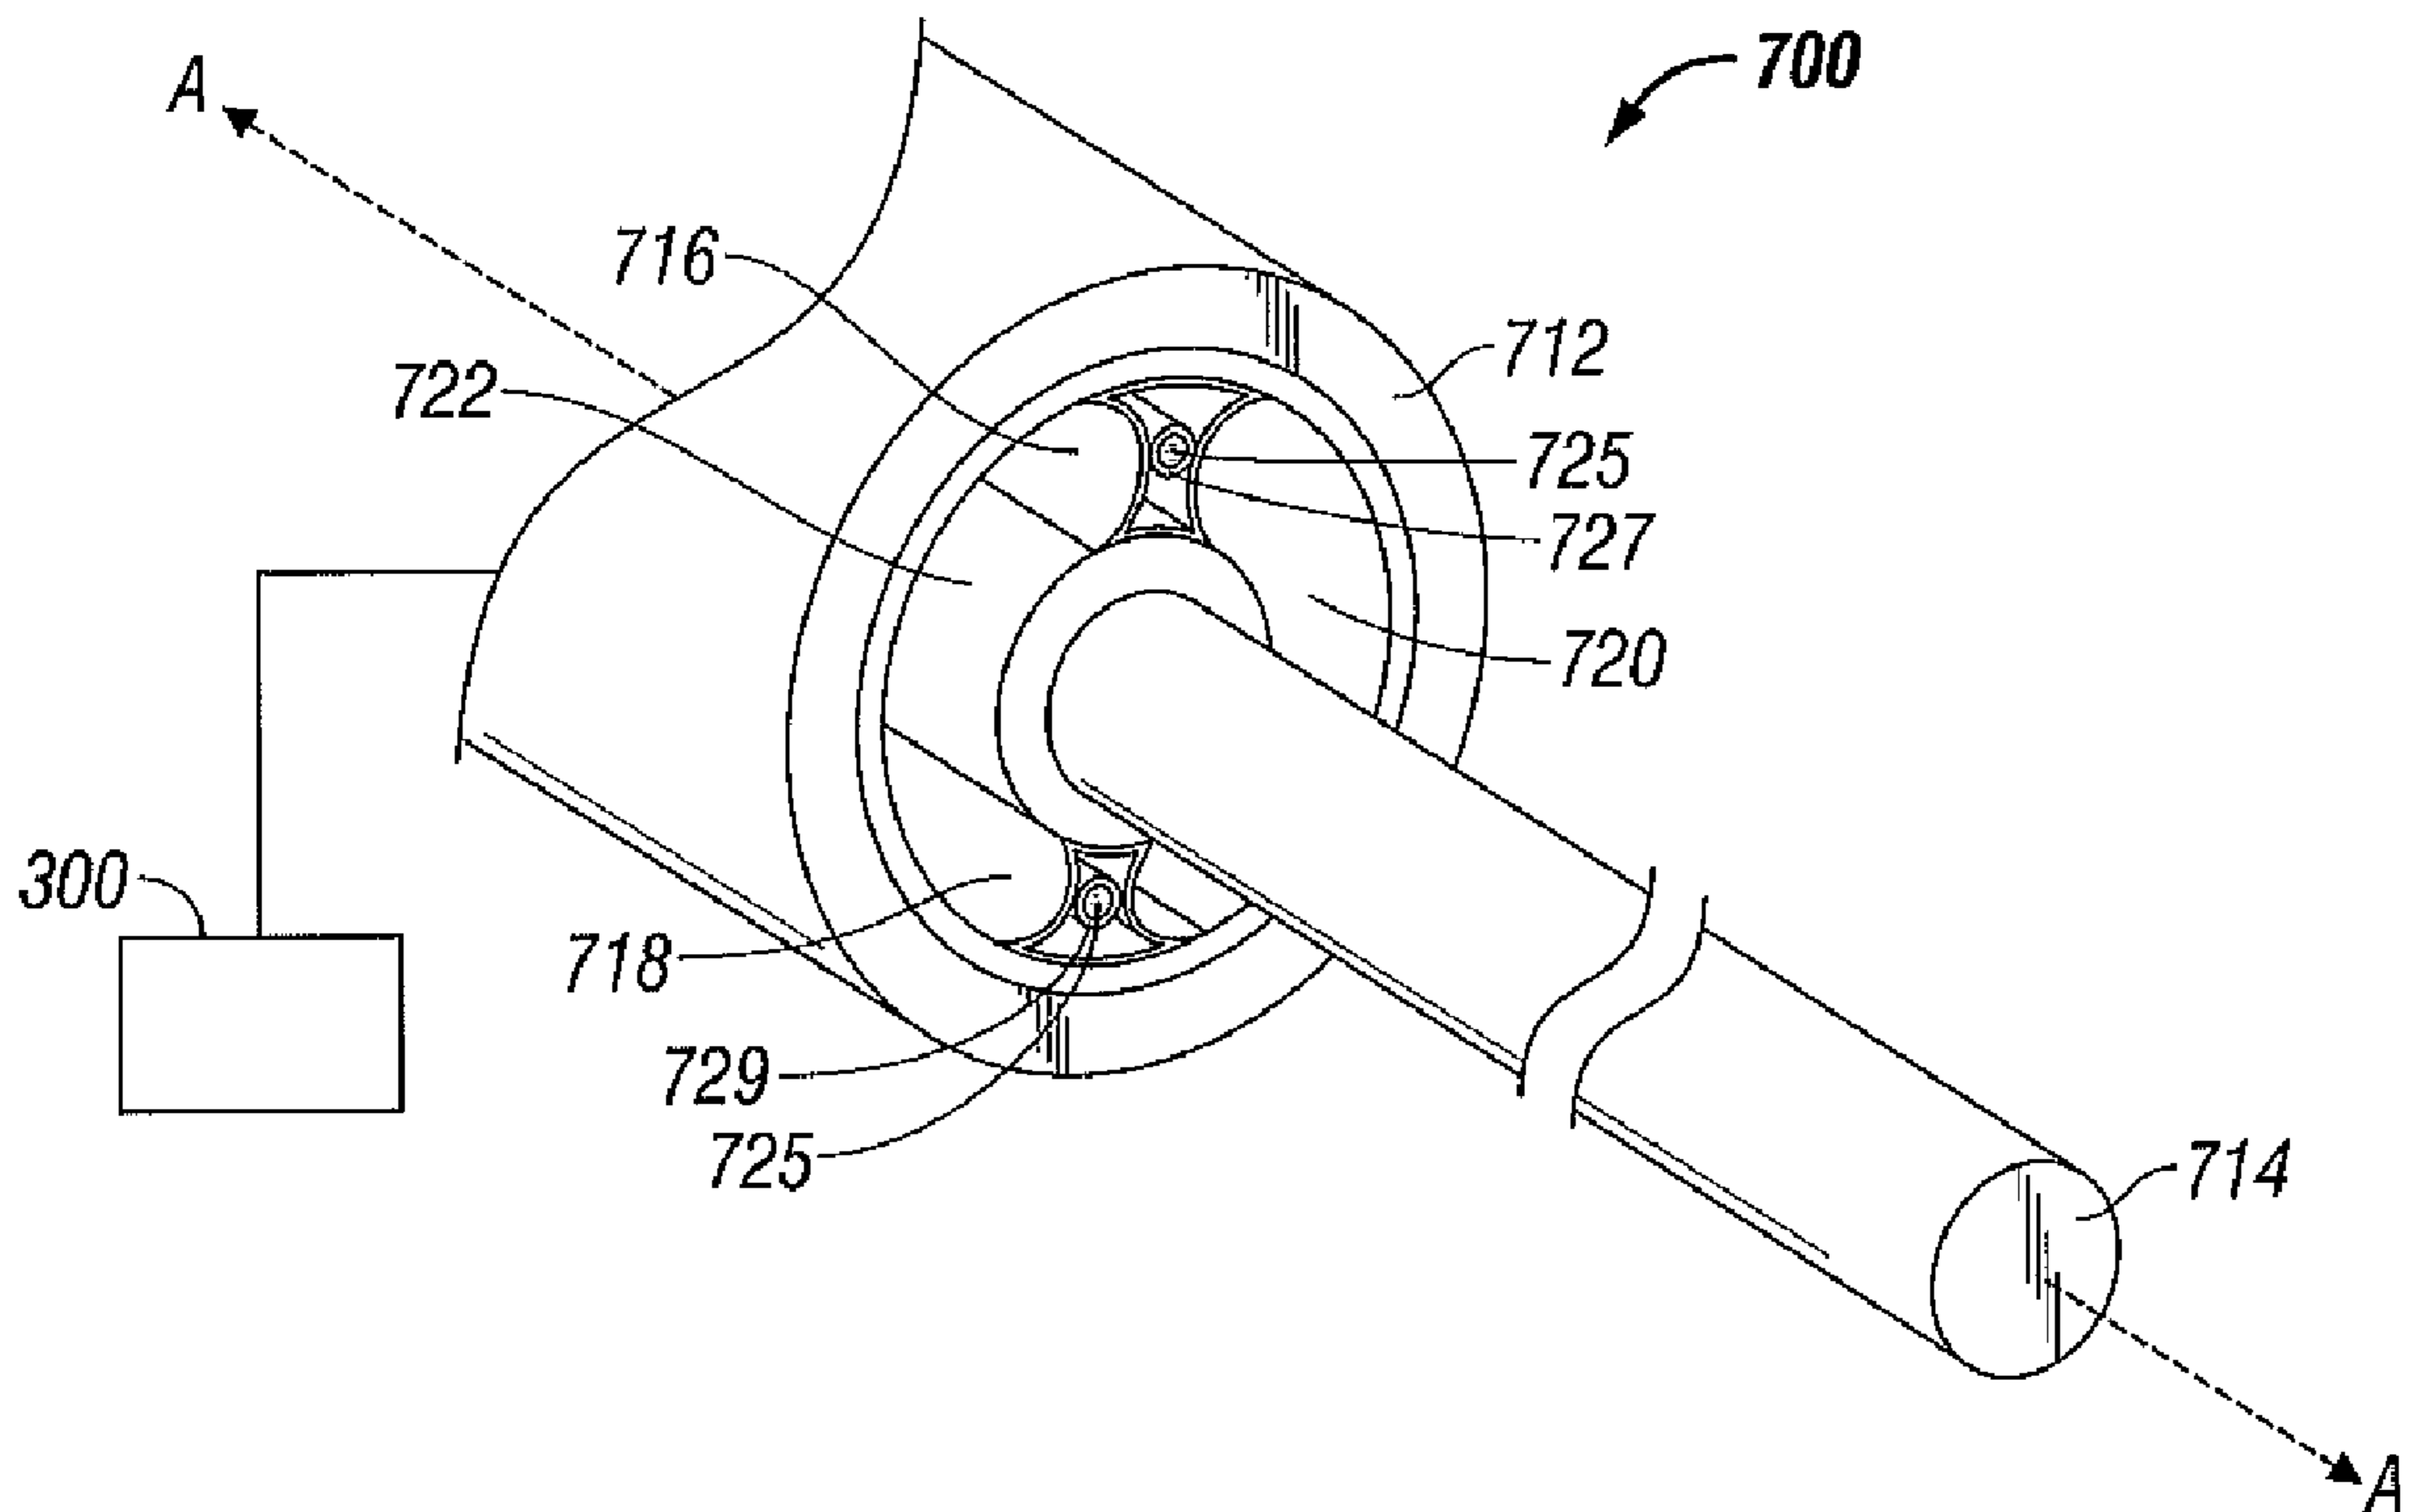


FIG. 7

1

THERMALLY TUNED COAXIAL CABLE FOR MICROWAVE ANTENNAS

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of priority to U.S. Provisional Patent Application Ser. No. 61/023,029, titled "THERMALLY TUNED COAXIAL CABLE FOR MICROWAVE ANTENNAS" filed Jan. 23, 2008 by Kenlyn Bonn, which is incorporated by reference herein.

BACKGROUND

1. Technical Field

The present disclosure relates generally to microwave antennas. More particularly, the present disclosure relates to thermally tuning coaxial cables for microwave antennas.

2. Background of Related Art

Microwave antennas are used in many applications. For example, medical microwave ablation antennas are used by surgeons. In fact, ablation devices utilizing DC shock, radio frequency (RF) current, ultrasound, microwave, direct heat, or lasers have been introduced and employed to various degrees to ablate biological tissues. Ablation devices may be used in open surgical procedures or are sometimes inserted into catheter devices in order to perform laparoscopic ablation procedures. The catheter incorporating the ablation device is generally inserted into a major vein or artery or through a body cavity. These catheters are then guided to a targeted location in the body (e.g., organ) by manipulating the catheter from the insertion point or the natural body orifice.

During ablation, the dielectric constant of the tissue changes as more water is boiled off and tissue desiccation occurs. The changing value of the dielectric constant alters the antenna's ability to match the originally designed impedance of the antenna. In addition, during microwave ablation in tissue, the impedance of the tissue varies during the course of ablation. This occurrence directly corresponds to how much energy has been deposited into the tissue during the ablation, resulting in temperature increases at the ablation site.

The impedance in the coaxial cable is typically related to the concentricity of the inner conductor in relationship to the outer conductor. In ablation procedures, however, conventional antenna designs only allow for an initial impedance match and as ablation occurs, the increase in mismatch between the tuning point of the antenna and the ablated tissue reduces the efficiency of the energy deposition in the tissue.

SUMMARY

The present disclosure relates to a coaxial cable. The coaxial cable includes an outer conductor and an inner conductor adapted to connect to an energy source for treating tissue, and first and second dielectric materials disposed between the inner conductor and the outer conductor which position the inner conductor relative to the outer conductor in general concentric relation thereto. The first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion.

In another embodiment, a coaxial cable also includes one or more dielectric spacer(s) disposed between the inner conductor and the outer conductor. The dielectric spacer(s) include first and second dielectric materials disposed between the inner conductor and the outer conductor, which position the inner conductor relative to the outer conductor in general

2

concentric relation thereto. The first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion.

5 In an example embodiment, a heating element is disposed within the dielectric material and is adapted to connect to an energy source for controlling the temperature thereof. The heating element heats the dielectric material to cause thermal expansion thereof.

10 The present disclosure also relates to a method for controlling the impedance of coaxial cable used to treat tissue, the method includes the steps of: providing an outer conductor and an inner conductor adapted to connect to an energy source for treating tissue. The first and second dielectric materials are disposed between the inner conductor and the outer conductor and position the inner conductor relative to the outer conductor in general concentric relation thereto. The first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion. The method also includes the steps of energizing the cable and determining the impedance of the inner conductor, and regulating the change of impedance of the inner conductor by selectively heating at least one of the first and second dielectric materials causing thermal expansion thereof to move the inner conductor relative to the outer conductor to change the impedance of the coaxial cable.

Thus, by using dielectric cores of varying thermal expansion values, it is possible to force the eccentricity of the inner conductor of the coaxial cable on-line or off-line effectively changing the coaxial cable's impedance value.

BRIEF DESCRIPTION OF THE DRAWINGS

35 Various embodiments of the present disclosure are described herein with reference to the drawings wherein:

FIG. 1A is a front, perspective view of a centrally-disposed coaxial cable having an inner conductor held by two materials having different coefficient of thermal expansion values, in accordance with an embodiment of the present disclosure;

FIG. 1B is a front, perspective view of an off-center coaxial cable having an inner conductor held by two materials having different coefficient of thermal expansion values, in accordance with another embodiment of the present disclosure;

FIG. 1C is a schematically-illustrated, cross-sectional view of the coaxial cable of FIG. 1A;

FIG. 1D is a schematically-illustrated, cross-sectional view of the coaxial cable of FIG. 1B;

50 FIG. 2A is front, perspective view of an off-centered coaxial cable having an inner conductor held by two materials having different coefficient of thermal expansion values, in accordance with another embodiment of the present disclosure;

FIG. 2B is a front, perspective view of a centrally disposed coaxial cable having an inner conductor held by two materials having different coefficient of thermal expansion values, in accordance with another embodiment of the present disclosure;

FIG. 2C is a schematically-illustrated, cross-sectional view of the coaxial cable of FIG. 2B;

FIG. 2D is a schematically-illustrated, cross-sectional view of the coaxial cable of FIG. 2A;

65 FIG. 3 is a schematically illustrated, cross-sectional view of a coaxial cable having an inner conductor held by one or more spacers being composed of one or more materials hav-

3

ing different coefficient of thermal expansion values, in accordance with another embodiment of the present disclosure;

FIG. 4A is a front, perspective view of an off-centered coaxial cable having an inner conductor and a plurality of resistive heating elements in each of two or more materials having different coefficient of thermal expansion values, in accordance with another embodiment of the present disclosure;

FIG. 4B is a front, perspective view of a centrally disposed coaxial cable having an inner conductor and a plurality of resistive heating elements in each of two or more materials having different coefficient of thermal expansion values, in accordance with another embodiment of the present disclosure;

FIG. 5A is a schematically illustrated cross-sectional view of an off-centered coaxial cable having an inner conductor and a plurality of resistive heating elements in one material having one coefficient of thermal expansion value, in accordance with another embodiment of the present disclosure;

FIG. 5B is a front, perspective view of a centrally disposed coaxial cable having an inner conductor and a plurality of resistive heating elements in one material having one coefficient of thermal expansion value, in accordance with another embodiment of the present disclosure;

FIG. 6 is a front, perspective view of a coaxial cable having an inner conductor with a shape memory alloy, in accordance with another embodiment of the present disclosure; and

FIG. 7 is a front, perspective view of a centrally-disposed coaxial cable having an inner conductor held by two materials having different coefficient of thermal expansion values with a fluid circulated therethrough for regulating the thermal expansion of the two materials in accordance with another embodiment of the present disclosure.

DETAILED DESCRIPTION

To achieve the foregoing and other objects of the present disclosure, methods and devices pertaining to the microwave antennas are disclosed. In general, the present disclosure pertains to a coaxial cable assembly and, in one embodiment, to a surgical device including the coaxial cable assembly. The surgical device generally includes an ablative energy source and an ablative energy delivery device coupled to the ablative energy source. The ablative energy delivery device is configured to deliver ablative energy sufficiently strong enough to cause tissue ablation. In most embodiments, the ablative energy is formed from electromagnetic energy in the microwave frequency range. Other applications are contemplated by the present disclosure, such as telecommunications or other suitable applications in which microwave antennas are utilized.

Particular embodiments of the present disclosure are described hereinbelow with reference to the accompanying drawings. In the following description, well-known functions or constructions are not described in detail to avoid obscuring the present disclosure in unnecessary detail. Those skilled in the art will understand that the present disclosure may be adapted for use with either an endoscopic instrument or an open instrument.

While the present disclosure is susceptible to embodiments in many different forms, there is shown in the drawings and will be described herein in detail one or more embodiments of the present disclosure. However, the present disclosure is to be considered an exemplification of the principles of the present disclosure, and the embodiment(s) illustrated is/are

4

not intended to limit the spirit and scope of the present disclosure and/or the claims herein.

With reference to the drawings, the coaxial cable of the particular embodiments of the present disclosure are shown. The cable may be of any suitable length, and the figures are not intended to limit the length of the cable to a specific length illustrated or any specific length. Instead, only a representative portion or section of cable is illustrated.

Referring to the embodiment of FIGS. 1A and 1B, the coaxial cable 10 includes an outer conductor 12, an inner conductor 14, a first material 16, a second material 18, a first air gap 20, and a second air gap 22. The inner conductor 14 is connected to an external power source 300.

The coaxial cable 10 may be rigid, rigid-but shapeable or flexible. The coaxial cable 10 may be chosen from commercially available standards and is generally designed with a characteristic impedance of 50 Ohms. In addition, one side of the coaxial cable 10 may be coupled to a power supply 300. Also, the other side of the coaxial cable 10 may be coupled to an antenna (not shown) in any suitable manner.

The outer conductor 12 is arranged to be generally concentric with respect to the inner conductor 14. However, the concentric relationship may be configured to meet a particular purpose as explained in more detail below. Inner conductor 14 is a central conductor used for transmitting signals and is typically held relative to the outer conductor 12 by first material 16 and second material 18. In one embodiment, the first material 16 holds the inner conductor 14, whereas the second material 18 supports the first material 16 without contacting the inner conductor 14. In other words, only one material contacts the inner conductor 14.

In the illustrated embodiment, the first material 16 and the second material 18 define first and second air gaps 20, 22 between the inner surface of the outer conductor 12 and the outer surface of the inner conductor 14. The first air gap 20 separates a first portion of the first material 16 and a first portion of the second material 18. The second air gap 22 separates a second portion of the first material 16 with a second portion of the second material 18.

The inner conductor 14 has a significant effect on the coaxial cable's 10 properties, such as the cable's 10 impedance and attenuation characteristics. The impedance on the coaxial cable 10 is related to the concentricity of the inner conductor 14 in relationship to the outer conductor 12. In the first embodiment, a thermal increase to the coaxial cable 10 is used to alter the alignment concentricity of the inner conductor 14 in a manner that would better match a change in tissue impedance. The coaxial cable 10 in the antenna (not shown) would start with an initial impedance match to a transmission line interface that would gradually taper along the length of the antenna toward a desired impedance with either the addition or the subtraction of heat. The taper could be controlled thermally through additional features, such as a cooling jacket or cooling channels.

FIGS. 1A and 1C illustrate the inner conductor 14 in a centered position within the coaxial cable 10. As heat is applied, the inner conductor 14 is moved to an off-centered position due to the thermal expansion of material 18, as shown in FIGS. 1B and 1D. As the tissue impedance changes, the alignment sensitivity of the cable 10 may be selectively changed (e.g., automatically or manually) such that the impedance of the cable 10 better matches the tissue impedance. One or more materials with different coefficients of thermal expansion may be utilized which mutually cooperate to tune the inner conductor 14 according to a desired setting, such as an ohmage setting.

5

FIGS. 2A and 2D show an off-centered coaxial cable **110** and FIGS. 2B and 2C show a centrally disposed coaxial cable **110** having an inner conductor held by two materials having different coefficient of thermal expansion values. The coaxial cable **110** includes an outer conductor **112**, an inner conductor **114**, a first material **116** and a second material **118**. The inner conductor **114** is connected to an external power source **300**.

The first material **116** has a first coefficient of thermal expansion value and the second material **118** has a second coefficient of thermal expansion value, the first and second coefficient of thermal expansion values being different. During heat transfer, the energy that is stored in the intermolecular bonds between atoms changes. When the stored energy increases, so does the length of the molecular bond. As a result, materials typically expand in response to heating and contract on cooling. This response to temperature change is expressed as the materials coefficient of thermal expansion. The coefficient of thermal expansion is used in two ways: (1) as a volumetric thermal expansion coefficient and (2) as a linear thermal expansion coefficient.

Therefore, when the temperature applied to the coaxial cable **110** changes, the first material **116** expands at a first rate/volume and the second material **118** expands at a second rate/volume. Typical materials used in coaxial cables include variations of PTFE, polyethylene (PE) blends and silica dioxides, however, nearly any thermo-set or thermoplastic with a low dielectric constant can be used in conjunction with another material of similar dielectric constant with a different coefficient of thermo-expansion. Typically, different polymer grades or blends result in varying material properties so determining the desired pair of materials would be a result of finding a matching mixture. The heat generated by the losses in the dielectric material in the cable can also be utilized to heat material enough to generate the differential in thermal expansion between the varying materials. A variety of different materials with different coefficient of thermal expansion values may be utilized, e.g., ABS Polymer Extruded, ABS Polymer Nylon Blend, PEEK Polyketone, PEKK Polyketone, Nylon PTFE Filled, Polycarbonate Extruded, LDPE (Polyethylene), Polyimide, PTFE Molded, Silica Aerogel and combinations thereof.

If the first material **116** expands due to a temperature increase, the second material **118** contracts due to the differing coefficient of thermal expansion values of the two materials **116**, **118**. As a result, as the ablation zone heats up, the difference in expansion between the two materials **116**, **118** would cause the inner conductor **114** to change alignment with the outer conductor **112**, e.g., move toward a centered position as illustrated in FIGS. 2B and 2C.

As can be appreciated, the materials **116**, **118** may be designed to selectively (e.g., either automatically or manually) align or misalign the inner conductor **114** relative to the outer conductor **112** for tuning and impedance matching purposes. In the embodiment, as seen in FIGS. 1A and 1B, the design could be made to start with the inner conductor **114** concentrically centered relative to outer conductor **112** and then moved off center when the temperature changes. As shown in FIGS. 2A and 2B, inner conductor **114** may be normally off-center relative to outer conductor **112**, and as the temperature increases, the inner conductor **114** moves toward the concentric center of the coaxial cable **110** when one of the materials **116**, **118** is heated.

The system described in regard to FIGS. 1A-2B may include an electrosurgical generator **300** having a microprocessor and sensor circuitry (not shown) that continually monitors tissue impedance and measures offset impedance. The

6

sensor circuitry may also continually monitor the position of the inner conductor **114** of a coaxial cable **110** with respect to a desired coaxial position (e.g., a center position). The monitor may be operably coupled to a mechanism (shape memory alloy, heat resistive element) as explained in more detail below) for regulating the thermal expansion of at least one of the first and second dielectric materials **116**, **118** to position the inner conductor **114** relative to the outer conductor **112** to change the impedance of the inner conductor **114**. The microprocessor or the circuitry may also be configured to compare the inner conductor positioning to a predetermined center position. If the inner conductor is positioned above or below the predetermined center position, one or more materials **116**, **118** surrounding the inner conductor are heated or moved to re-position the inner conductor **114** to a desired position, and the microprocessor reports such findings to a user control or maintains this data for subsequent use.

FIG. 3 is a schematically illustrated cross-sectional view of a coaxial cable **210** having an inner conductor **214** held by one or more spacers **230**, **232**, **234** being composed of one or more materials having different coefficient of thermal expansion values. In FIG. 3, the coaxial cable **210** includes an outer conductor **212**, an inner conductor **214**, a first material **216**, a second material **218**, a first spacer **230**, a second spacer **232** and a third spacer **234**. The inner conductor **214** is connected to an external power source **300**.

The first, second, and third spacers **230**, **232**, **234** maintain a desired position (e.g., a center position) for the inner conductor **214** for at least a partial length of the coaxial cable **210**. Each of the spacers **230**, **232**, **234** may have the same or a different width, and each may be composed of one material or two or more materials. Also, the material used for each spacer may be different. For example, a first spacer **230** may be composed of a first material **216** and a second material **218**, whereas the second and third spacers **232**, **234** may be composed of one material.

FIG. 4A is a schematically illustrated cross-sectional view of an off-centered coaxial cable **310** and FIG. 4B is a schematically illustrated cross-sectional view of a centrally disposed coaxial cable **310** having an inner conductor and a plurality of resistive heating elements in each of two or more materials having different coefficient of thermal expansion values. In FIGS. 4A and 4B, the coaxial cable **310** includes an outer conductor **312**, an inner conductor **314**, a first material **316**, a second material **318**, first resistive heating elements **340** and second resistive heating elements **342**.

FIG. 4A illustrates the inner conductor **314** in an off-centered position within the coaxial cable **310**. As heat is applied via the heating resistive elements **340**, **342** shown in FIG. 4B, the inner conductor **314** moves to a centered position due to the thermal expansion of material **318**. As the tissue impedance changes, the alignment sensitivity of the cable **310** may be selectively changed (e.g., automatically or manually) such that the impedance of the cable **310** better matches the tissue impedance. One or more materials may be utilized to tune the inner conductor **314** according to a desired setting, such as an ohmage setting.

A plurality of first resistive heating elements **340** may be positioned in first material **316** and a plurality of second resistive heating elements **342** may be positioned in second material **318**. The first and second resistive heating elements **340**, **342** convert electricity into heat. Electrical current running through the elements encounter resistance, thus resulting in heating of the element. Resistive heating elements **340**, **342** may be made from Nichrome which has a relatively high resistance and does not break down or oxidize in air at useful temperature ranges. First and second resistive heating ele-

ments **340**, **342** may also be positioned in parallel to the inner conductor **314**, at various lengths from the inner conductor **314**, and in various widths. The temperature of each of the plurality of heating elements **340**, **342** may be selectively controllable to position the inner conductor **314** relative to the outer conductor **312** and the plurality of heating elements **340**, **342** may be disposed in a concentric array relative to the inner conductor **314**.

FIG. **5A** is a schematically illustrated cross-sectional view of an off-centered coaxial cable **410** and FIG. **5B** is a schematically illustrated cross-sectional view of a centrally disposed coaxial cable **410**. In FIGS. **5A** and **5B**, the coaxial cable **410** includes an outer conductor **412**, an inner conductor **414**, a dielectric material **416**, and one or more resistive heating elements **440**. In contrast to FIGS. **4A** and **4B**, only one dielectric material **416** is used to surround the entire length of the inner conductor **414**. The dielectric material **416** includes one or more resistive heating elements **440** in parallel to the inner conductor **414** along the length of the cable **410**. More particularly, the resistive heating elements **440** are positioned in parallel to the inner conductor **414**, at various lengths along the inner conductor **414**, and in various widths.

FIG. **5A** illustrates the inner conductor **414** in an off-centered position within the dielectric material **416**. As heat is applied, the inner conductor **414** is moved to a desired position (e.g., a center position) due to the thermal expansion of dielectric material **416** and due to first resistive heating element **440b** being heated to expand the dielectric material **416** in a given direction. Any member or combination of heating elements **440a-440e** may be utilized to move the inner conductor **414** for tuning purposes. As the tissue impedance changes, the alignment sensitivity of the cable **410** may be selectively changed (e.g., automatically or manually) such that the impedance of the cable **410** better matches the tissue impedance.

FIG. **6** is a schematically illustrated cross-sectional view of a coaxial cable having an inner conductor with a shape memory alloy **550** in accordance with another embodiment of the present disclosure. In FIG. **6**, the coaxial cable **510** includes an outer conductor **512**, an inner conductor **514**, a dielectric material **516** and a shape memory alloy **550**.

The shape memory alloy **550** is, for example, positioned in proximity to the inner conductor **514**. One or more shape memory alloys **550** may be positioned along the length of the coaxial cable **510** in predetermined distance from each other.

Shape memory alloys (SMAs) are a family of alloys having anthropomorphic qualities of memory and trainability and are particularly well suited for use with medical instruments. SMAs have been applied to such items as actuators for control systems, steerable catheters and clamps. One of the most common SMAs is Nitinol which can retain shape memories for two different physical configurations and changes shape as a function of temperature. Recently, other SMAs have been developed based on copper, zinc and aluminum and have similar shape memory retaining features.

SMAs undergo a crystalline phase transition upon applied temperature and/or stress variations. A particularly useful attribute of SMAs is that after it is deformed by temperature/stress, it can completely recover its original shape on being returned to the original temperature. The ability of an alloy to possess shape memory is a result of the fact that the alloy undergoes a reversible transformation from an austenitic state to a martensitic state with a change in temperature/stress. This transformation is referred to as a thermoelastic martensitic transformation.

Under normal conditions, the thermoelastic martensitic transformation occurs over a temperature range which varies

with the composition of the alloy, itself, and the type of thermal-mechanical processing by which it was manufactured. In other words, the temperature at which a shape is “memorized” by an SMA is a function of the temperature at which the martensite and austenite crystals form in that particular alloy. For example, Nitinol alloys can be fabricated so that the shape memory effect will occur over a wide range of temperatures, e.g., -270° to $+100^{\circ}$ Celsius. Many SMAs are also known to display stress-induced martensite (SIM) which occurs when the alloy is deformed from its original austenitic state to a martensitic state by subjecting the alloy to a stress condition.

As a result, when heat is applied to the coaxial cable **510**, the inner conductor **514** tends to move from its desired position within the coaxial cable **510**. SMA **550**, which is embedded within a material **516** having a certain coefficient of thermal expansion and which is located in a close proximity to the inner conductor **514** may move the inner conductor **514** back to its desired position (e.g., a center position) within the coaxial cable **510**. SMA **550** can recover from large amounts of bending and torsional deformations, due to the application of heat, as well as small amounts of strain. Provided the deformations are within recoverable ranges, the process of deformation and shape recovery can be repeated millions of times. As a result, the SMA **550** located within the material **516** can repeatedly move the inner conductor **514** back to a desired position (e.g., a centered position). Moreover, as can be appreciated, the material **516** may be designed to selectively (e.g., either automatically or manually) align or misalign the inner conductor **514** relative to the outer conductor **512** for tuning and impedance matching purposes.

Consequently, the embodiments of the present disclosure allow for improved antenna impedance matching for controlling tissue impedance of a microwave antenna during an ablation procedure via a thermally tuned coaxial cable. The embodiments further include changing the impedance of the coaxial cable for allowing greater flexibility in designing microwave antennas. By having a varying impedance of the coaxial cable in the antenna tuned to change with the increase/decrease in temperature, tissue impedance changes, and thus, the antenna may deposit a greater amount of energy over the entire course of the ablation procedure. By using dielectric cores of varying thermal expansion values, it is possible to force the eccentricity of the inner conductor of the coaxial cable on-line or off-line, thus effectively changing the coaxial cable’s impedance value.

In addition, FIGS. **1A-2D** illustrate two materials **16**, **18** within the spacing between the inner surface of the outer conductor **12** and the outer surface of the inner conductor **14** including two air spaces or gaps **20**, **22**. However, one skilled in the art may use more than two materials within the spacing between the inner surface of the outer conductor **12** and the outer surface of the inner conductor **14** and more than two air gaps. For example, one skilled in the art may be motivated to use three or more materials, each with a different coefficient of thermal expansion value in a triangular configuration with three or more air gaps separating the materials. In addition, one skilled in the art may be motivated to use two materials in a checkered pattern or any other type of intertwined pattern with one or more air gaps in order to center or off-center the inner conductor **14** of the coaxial cable **10** as needed to tune or match the tissue impedance.

Further, in FIGS. **1A-6** there may be one or more mechanisms that regulate the thermal expansion of at least one of the first and second dielectric materials **16**, **18** to position the inner conductor **14** relative to the outer conductor **12** to change the impedance of the inner conductor **14**.

FIG. 7 shows another embodiment according to the present disclosure wherein the coaxial cable 700 includes an outer conductor 712 arranged to be generally concentric with respect to the inner conductor 714 used for transmitting signals. Inner conductor 714 is held relative to the outer conductor 712 by first material 716 and second material 718 only one of which contacts inner conductor 714. First material 716 and the second material 718 define first and second air gaps 720 and 722, respectively, between the inner surface of the outer conductor 712 and the outer surface of the inner conductor 714. A fluid 725 is circulated within one or both the first and second dielectric materials 716, 718 via conduits 727 and 729 defined respectively therein. The relative temperature of the fluid 725 may be selectively controllable via circuitry controlled by the generator 300 to regulate thermal expansion of one or both the first and second dielectric materials 716, 718 to position the inner conductor 714 relative to the outer conductor 712 to change the impedance of the inner conductor 714. The fluid 725 may optionally or alternatively be disposed between the first and second dielectric materials 716, 718 and be controlled in a similar manner.

While several embodiments of the disclosure have been shown in the drawings and/or discussed herein, it is not intended that the disclosure be limited thereto, as it is intended that the disclosure be as broad in scope as the art will allow and that the specification be read likewise. Therefore, the above description should not be construed as limiting, but merely as examples of particular embodiments. Those skilled in the art will envision other modifications within the scope and spirit of the claims appended hereto.

What is claimed is:

1. A coaxial cable, comprising:
an outer conductor and an inner conductor adapted to connect to an energy source; and
first and second dielectric materials disposed between the inner conductor and the outer conductor that position the inner conductor relative to the outer conductor in a first position, wherein the first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion.
2. The coaxial cable according to claim 1, wherein the first and second dielectric materials are thermally expandable and contractible to position the inner conductor relative to the outer conductor from the first position to a second position different from the first position.
3. The coaxial cable according to claim 1, wherein the first and second dielectric materials are at least one of thermally expandable and contractible to position the inner conductor relative to the outer conductor from the first position wherein the inner conductor is concentrically aligned with the outer conductor to a second position wherein the inner conductor is not concentrically aligned with the outer conductor.
4. The coaxial cable according to claim 1, wherein the first dielectric material is selected from the group consisting of ABS Polymer Extruded, ABS Polymer Nylon Blend, PEKK Polyketone, PEEK Polyketone, Nylon PTFE Filled, Polycarbonate Extruded, LDPE (Polyethylene), Polyimide, PTFE Molded, Silica Aerogel and combinations thereof.
5. The coaxial cable according to claim 1, wherein the second dielectric material is selected from the group consisting of ABS Polymer Extruded, ABS Polymer Nylon Blend, PEKK Polyketone, PEEK Polyketone, Nylon PTFE Filled,

Polycarbonate Extruded, LDPE (Polyethylene), Polyimide, PTFE Molded, Silica Aerogel and combinations thereof.

6. The coaxial cable according to claim 1, wherein the first and second dielectric materials define at least one space disposed therebetween.

7. The coaxial cable according to claim 1, further comprising at least one of a shape memory alloy and a resistive heating element operatively associated with at least one of the first and second dielectric materials for regulating the thermal expansion of at least one of the first and second dielectric materials to position the inner conductor relative to the outer conductor.

8. The coaxial cable according to claim 1, wherein a fluid is disposed between the first and second dielectric materials, the relative temperature of the fluid being selectively controllable to regulate thermal expansion of at least one of the first and second dielectric materials to position the inner conductor relative to the outer conductor.

9. The coaxial cable according to claim 1, wherein at least one heating element is disposed within at least one of the first and second dielectric materials, the relative temperature of the heating element being selectively controllable to regulate thermal expansion of at least one of the first and second dielectric materials to position the inner conductor relative to the outer conductor.

10. The coaxial cable according to claim 1, wherein the first dielectric material holds the inner conductor and the second dielectric material mechanically supports the first material.

11. The coaxial cable according to claim 1, wherein the energy source includes sensor circuitry that monitors at least one of the inner and outer conductors for determining the position of the inner conductor relative to the outer conductor.

12. The coaxial cable according to claim 11, wherein the sensor circuitry is operably coupled to a means for regulating the thermal expansion of at least one of the first and second dielectric materials to position the inner conductor relative to the outer conductor to change the impedance of the inner conductor, the means for regulating including at least one of a shape memory alloy, a heat resistive element and a temperature controllable fluid.

13. A coaxial cable, comprising:
an outer conductor and an inner conductor adapted to connect to an energy source; and
at least one dielectric spacer disposed between the outer conductor and an inner conductor, the dielectric spacer including first and second dielectric materials disposed between the inner conductor and the outer conductor that position the inner conductor relative to the outer conductor in a first position, wherein the first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion.

14. The coaxial cable according to claim 13 further comprising a plurality of dielectric spacers spaced relative to one another along a length of the cable.

15. A coaxial cable, comprising:
an outer conductor and an inner conductor adapted to connect to an energy source;
at least one dielectric material disposed between the outer conductor and an inner conductor, wherein the dielectric material is thermally expandable to position the inner conductor relative to the outer conductor from a first

11

position wherein the inner conductor is not concentrically aligned with the outer conductor to a second position wherein the inner conductor is more concentrically aligned with the outer conductor; and

at least one heating element disposed within the dielectric material adapted to connect to an energy source for controlling the temperature thereof.

16. A coaxial cable according to claim **15** further comprising a plurality of heating elements disposed within the dielectric material, the temperature of each of the plurality of heating elements being selectively controllable to position the inner conductor relative to the outer conductor.

17. A coaxial cable according to claim **16** wherein the plurality of heating elements is disposed in a concentric array relative to the inner conductor.

18. A coaxial cable according to claim **15**, wherein the generator further comprises sensor circuitry which monitors the position of the inner conductor within the coaxial cable.

19. A method for controlling the impedance of a coaxial cable, the method comprising:

12

providing:

an outer conductor and an inner conductor;

first and second dielectric materials disposed between the inner conductor and the outer conductor, wherein the first dielectric material has a first coefficient of thermal expansion and the second dielectric material has a second coefficient of thermal expansion different from the first coefficient of thermal expansion;

energizing the cable;

determining an impedance of the inner conductor; and causing at least one of the first and second dielectric materials to thermally expand or contract to move the inner conductor relative to the outer conductor to change the impedance of the coaxial cable.

20. A method according to claim **19** wherein the impedance of the coaxial cable is substantially matched to the impedance of at least one of a microwave generator and a microwave probe.

* * * * *