

US007701209B1

(12) **United States Patent  
Green**

(10) **Patent No.:** US 7,701,209 B1  
(45) **Date of Patent:** Apr. 20, 2010

(54) **COILS FOR HORIZONTAL FIELD  
MAGNETIC RESONANCE IMAGING**

(75) Inventor: **Charles A. Green**, Holbrook, NY (US)

(73) Assignee: **Fonar Corporation**, Melville, NY (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 493 days.

4,664,275 A	5/1987	Kasai et al.
4,668,915 A	5/1987	Daubin et al.
4,672,346 A	6/1987	Miyamoto et al.
4,675,609 A	6/1987	Danby et al.
4,679,022 A	7/1987	Miyamoto et al.
4,707,663 A	11/1987	Minkoff et al.
4,766,378 A	8/1988	Danby et al.
4,767,160 A	8/1988	Mengshoel et al.

(21) Appl. No.: **10/998,395**

(22) Filed: **Nov. 29, 2004**

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 10/266,070, filed on Oct. 7, 2002, now abandoned.

(60) Provisional application No. 60/327,329, filed on Oct. 5, 2001, provisional application No. 60/342,832, filed on Dec. 20, 2001.

(51) **Int. Cl.**  
**G01V 3/00** (2006.01)

(52) **U.S. Cl.** ..... **324/307; 324/318**

(58) **Field of Classification Search** ..... **324/300-322;**  
**600/410-435**

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,810,254 A	5/1974	Utsumi et al.
4,407,292 A	10/1983	Edrich et al.
4,411,270 A	10/1983	Damadian
4,534,076 A	8/1985	Barge
4,534,358 A	8/1985	Young
D283,858 S	5/1986	Opsvik et al.
4,608,991 A	9/1986	Rollwitz
4,613,820 A	9/1986	Edelstein et al.
4,614,378 A	9/1986	Picou
4,629,989 A	12/1986	Riehl et al.
4,641,119 A	2/1987	Moore
4,651,099 A	3/1987	Vinegar et al.
4,663,592 A	5/1987	Yamaguchi et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

DE 3140225 A1 4/1983

(Continued)

**OTHER PUBLICATIONS**

Feng, et al., A New Phased Array Spine Coil for Vertical Field MRI System, Proc. Intl. Soc. Mag. Reson. Med. 11, 2003.

(Continued)

*Primary Examiner*—Brij B Shrivastav


*Assistant Examiner*—Dixomara Vargas

(74) *Attorney, Agent, or Firm*—Lerner, David, Littenberg, Krumholz & Mentlik, LLP

(57) **ABSTRACT**

Apparatus for performing magnetic resonance imaging are disclosed. In one aspect coil antennas for use with a horizontal field magnetic resonance imaging apparatus are placed in proximity to the scanning region to obtain magnetic resonance images. The coils are arranged in quadrature geometry and housed in a planar structure.

**8 Claims, 14 Drawing Sheets**

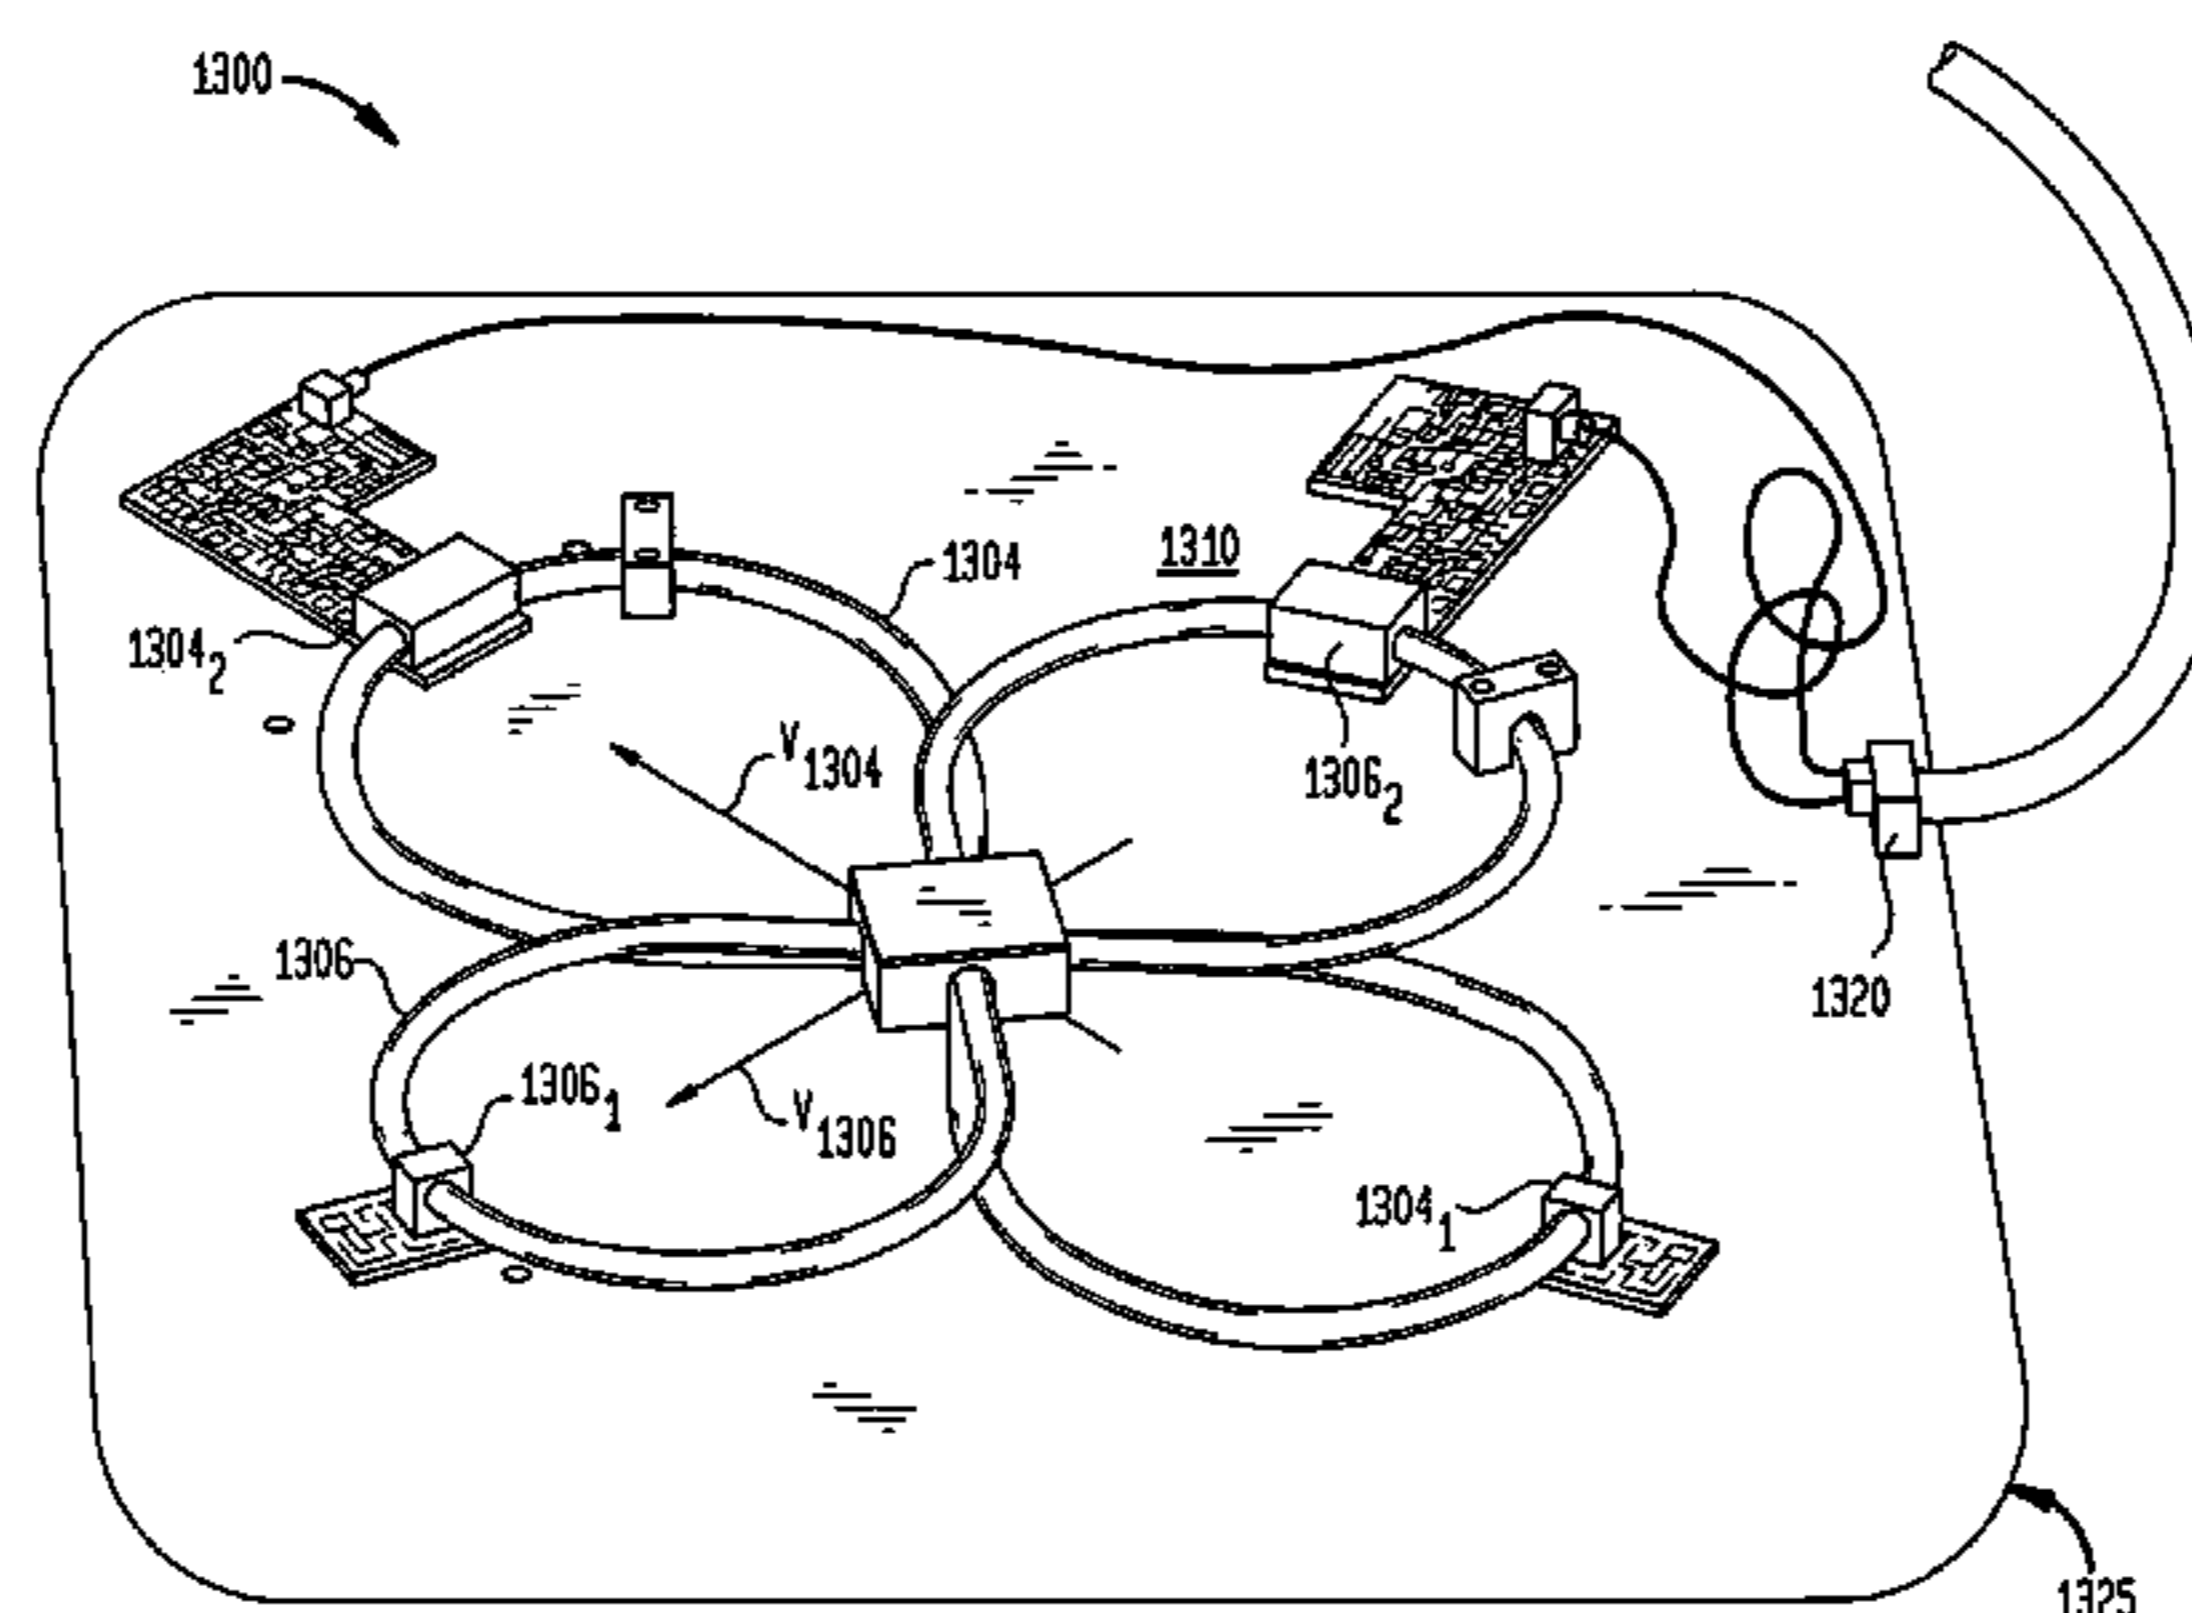

# US 7,701,209 B1

U.S. PATENT DOCUMENTS							
4,770,182	A	9/1988	Damadian et al.	5,666,056	A	9/1997	Cuppen et al.
4,777,464	A	10/1988	Takabatashi et al.	5,671,526	A	9/1997	Merlano et al.
4,816,765	A	3/1989	Boskamp	5,680,861	A	10/1997	Rohling
4,829,252	A	5/1989	Kaufman	5,682,098	A *	10/1997	Vij ..... 324/318
4,866,387	A	9/1989	Hyde et al.	5,735,278	A	4/1998	Hoult et al.
4,875,485	A	10/1989	Matsutani	5,743,264	A	4/1998	Bonutti
4,908,844	A	3/1990	Hasegawa	5,754,085	A	5/1998	Danby et al.
4,918,388	A *	4/1990	Mehdizadeh et al. .... 324/322	5,779,637	A	7/1998	Palkovich et al.
4,920,318	A	4/1990	Misic et al.	5,836,878	A	11/1998	Mock et al.
4,924,198	A	5/1990	Laskaris	5,862,579	A	1/1999	Blumberg et al.
4,943,774	A	7/1990	Breneman et al.	5,929,639	A *	7/1999	Doty ..... 324/318
4,968,937	A	11/1990	Akgun	5,951,474	A *	9/1999	Matsunaga et al. .... 600/422
4,985,678	A	1/1991	Gangarosa et al.	D417,085	S	11/1999	Kanwetz, II
5,008,624	A	4/1991	Yoshida	5,983,424	A	11/1999	Naslund
5,030,915	A	7/1991	Boskamp et al.	5,988,173	A	11/1999	Scruggs
5,050,605	A	9/1991	Eydelman et al.	6,008,649	A	12/1999	Boskamp et al.
5,061,897	A	10/1991	Danby et al.	6,011,396	A	1/2000	Eckels et al.
5,062,415	A	11/1991	Weatherby et al.	6,014,070	A	1/2000	Danby et al.
5,065,701	A	11/1991	Punt	6,023,165	A *	2/2000	Damadian et al. .... 324/318
5,065,761	A	11/1991	Pell	6,075,364	A	6/2000	Damadian et al.
5,081,665	A	1/1992	Kostich	6,122,541	A	9/2000	Cosman et al.
5,124,651	A	6/1992	Danby et al.	6,137,291	A *	10/2000	Szumowski et al. .... 324/318
5,134,374	A	7/1992	Breneman et al.	6,138,302	A	10/2000	Sashin et al.
5,153,517	A *	10/1992	Oppelt et al. .... 324/322	6,141,579	A	10/2000	Bonutti
5,153,546	A	10/1992	Laskaris	6,144,204	A	11/2000	Sementchenko et al.
5,155,758	A	10/1992	Vogl	6,150,819	A	11/2000	Laskaris et al.
5,162,768	A	11/1992	McDougall et al.	6,150,820	A	11/2000	Damadian et al.
5,171,296	A	12/1992	Herman	6,201,394	B1	3/2001	Danby et al.
5,194,810	A	3/1993	Breneman et al.	6,208,144	B1	3/2001	McGinley et al.
5,197,474	A	3/1993	Englund et al.	6,226,856	B1	5/2001	Kazama et al.
5,207,224	A	5/1993	Dickinson et al.	6,246,239	B1 *	6/2001	Krogmann et al. .... 324/318
5,221,165	A	6/1993	Goszczynski	6,246,900	B1	6/2001	Cosman et al.
5,221,902	A	6/1993	Jones et al.	6,249,121	B1 *	6/2001	Boskamp et al. .... 324/318
5,229,723	A	7/1993	Sakurai et al.	6,249,695	B1 *	6/2001	Damadian ..... 600/427
5,250,901	A	10/1993	Kaufman et al.	6,285,188	B1	9/2001	Sakakura et al.
5,251,961	A	10/1993	Pass	6,346,814	B1	2/2002	Carrozzi et al.
5,256,971	A	10/1993	Boskamp	6,357,066	B1	3/2002	Pierce
5,274,332	A	12/1993	Jaskolski	6,369,571	B1	4/2002	Damadian et al.
5,291,890	A	3/1994	Cline et al.	6,377,044	B1 *	4/2002	Burl et al. .... 324/307
5,304,932	A	4/1994	Carlson	6,385,481	B2	5/2002	Nose et al.
5,305,365	A	4/1994	Coe	6,411,088	B1	6/2002	Kuth et al.
5,305,749	A	4/1994	Li et al.	6,414,490	B1	7/2002	Damadian et al.
5,315,244	A	5/1994	Griebeler	6,424,854	B2	7/2002	Hayashi et al.
5,315,276	A	5/1994	Huson et al.	6,456,075	B1	9/2002	Damadian et al.
5,317,297	A	5/1994	Kaufman et al.	6,504,371	B1	1/2003	Damadian et al.
5,323,113	A *	6/1994	Cory et al. .... 324/318	6,549,800	B1	4/2003	Atalar et al.
5,349,956	A	9/1994	Bonutti	6,591,128	B1 *	7/2003	Wu et al. .... 600/422
5,382,904	A	1/1995	Pissanetzky	6,639,406	B1 *	10/2003	Boskamp et al. .... 324/318
5,382,905	A	1/1995	Miyata et al.	6,677,753	B1 *	1/2004	Danby et al. .... 324/318
5,386,447	A	1/1995	Siczek	6,792,257	B2	9/2004	Rabe et al.
5,394,087	A	2/1995	Molyneaux	6,801,038	B2	10/2004	Carrozzi et al.
5,412,363	A	5/1995	Breneman et al.	6,806,711	B2 *	10/2004	Reykowski ..... 324/318
5,436,607	A	7/1995	Chari et al.	6,850,064	B1	2/2005	Srinivasan
5,471,142	A	11/1995	Wang	6,882,149	B2	4/2005	Nitz et al.
5,473,251	A	12/1995	Mori	6,882,877	B2	4/2005	Bonutti
5,475,885	A	12/1995	Ishikawa	6,894,495	B2	5/2005	Kan
5,477,146	A	12/1995	Jones	6,954,069	B2 *	10/2005	Harvey et al. .... 324/318
5,490,513	A	2/1996	Damadian et al.	6,980,002	B1 *	12/2005	Petropoulos et al. .... 324/318
5,515,863	A	5/1996	Damadian	7,046,006	B2 *	5/2006	Creemers ..... 324/318
5,519,372	A	5/1996	Palkovich et al.	7,049,819	B2 *	5/2006	Chan et al. .... 324/319
5,548,218	A *	8/1996	Lu ..... 324/318	7,221,161	B2 *	5/2007	Fujita et al. .... 324/318
5,553,777	A	9/1996	Lampe	7,245,127	B2 *	7/2007	Feng et al. .... 324/318
5,566,681	A	10/1996	Manwaring et al.	7,348,778	B2 *	3/2008	Chu et al. .... 324/318
5,578,925	A	11/1996	Molyneaux et al.	7,474,098	B2 *	1/2009	King ..... 324/318
5,592,090	A	1/1997	Pissanetzky	2001/0029330	A1	10/2001	Nose et al.
5,606,970	A	3/1997	Damadian	2002/0013524	A1	1/2002	Hayashi et al.
5,621,323	A *	4/1997	Larsen ..... 324/318	2002/0032927	A1	3/2002	Dinkler
5,623,241	A	4/1997	Minkoff	2002/0101241	A1	8/2002	Chui
5,640,958	A	6/1997	Bonutti	2002/0123681	A1	9/2002	Zuk et al.
5,652,517	A	7/1997	Maki et al.	2002/0196021	A1	12/2002	Wang
5,654,603	A	8/1997	Sung et al.				

2003/0210049 A1 11/2003 Boskamp et al.

FOREIGN PATENT DOCUMENTS

JP	1242056	9/1989
JP	4-332531	11/1992
JP	62-26052	8/1994
JP	08-050843 A	2/1996
WO	WO-97/17896	5/1997

OTHER PUBLICATIONS

Guclu et al., A method for Preamplifier-Decoupling Improvement in Quadrature Phased-Array Coils, Journal of Magnetic Resonance Imaging, 19:255-258, 2004.

U.S. Appl. No. 08/978,084, filed Nov. 25, 1997.

U.S. Appl. No. 10/131,843, filed Apr. 25, 2002.

U.S. Appl. No. 09/718,946, filed Nov. 22, 2000.

Weis et al., Simulation of the influence of magnetic field inhomogeneity and distortion correction in MR imaging, vol. 8, No. 4, p. 483-489, 1990 (Abstract).

"The design and construction of high field-uniformity permanent magnet system for MRI" Feng, Z.X.; Jiang, X.H.; Han, S.; Magnetics, IEEE Transactions on vol. 28, Issue 1, Jan. 1992 pp. 641-643.

\* cited by examiner

FIG. 1

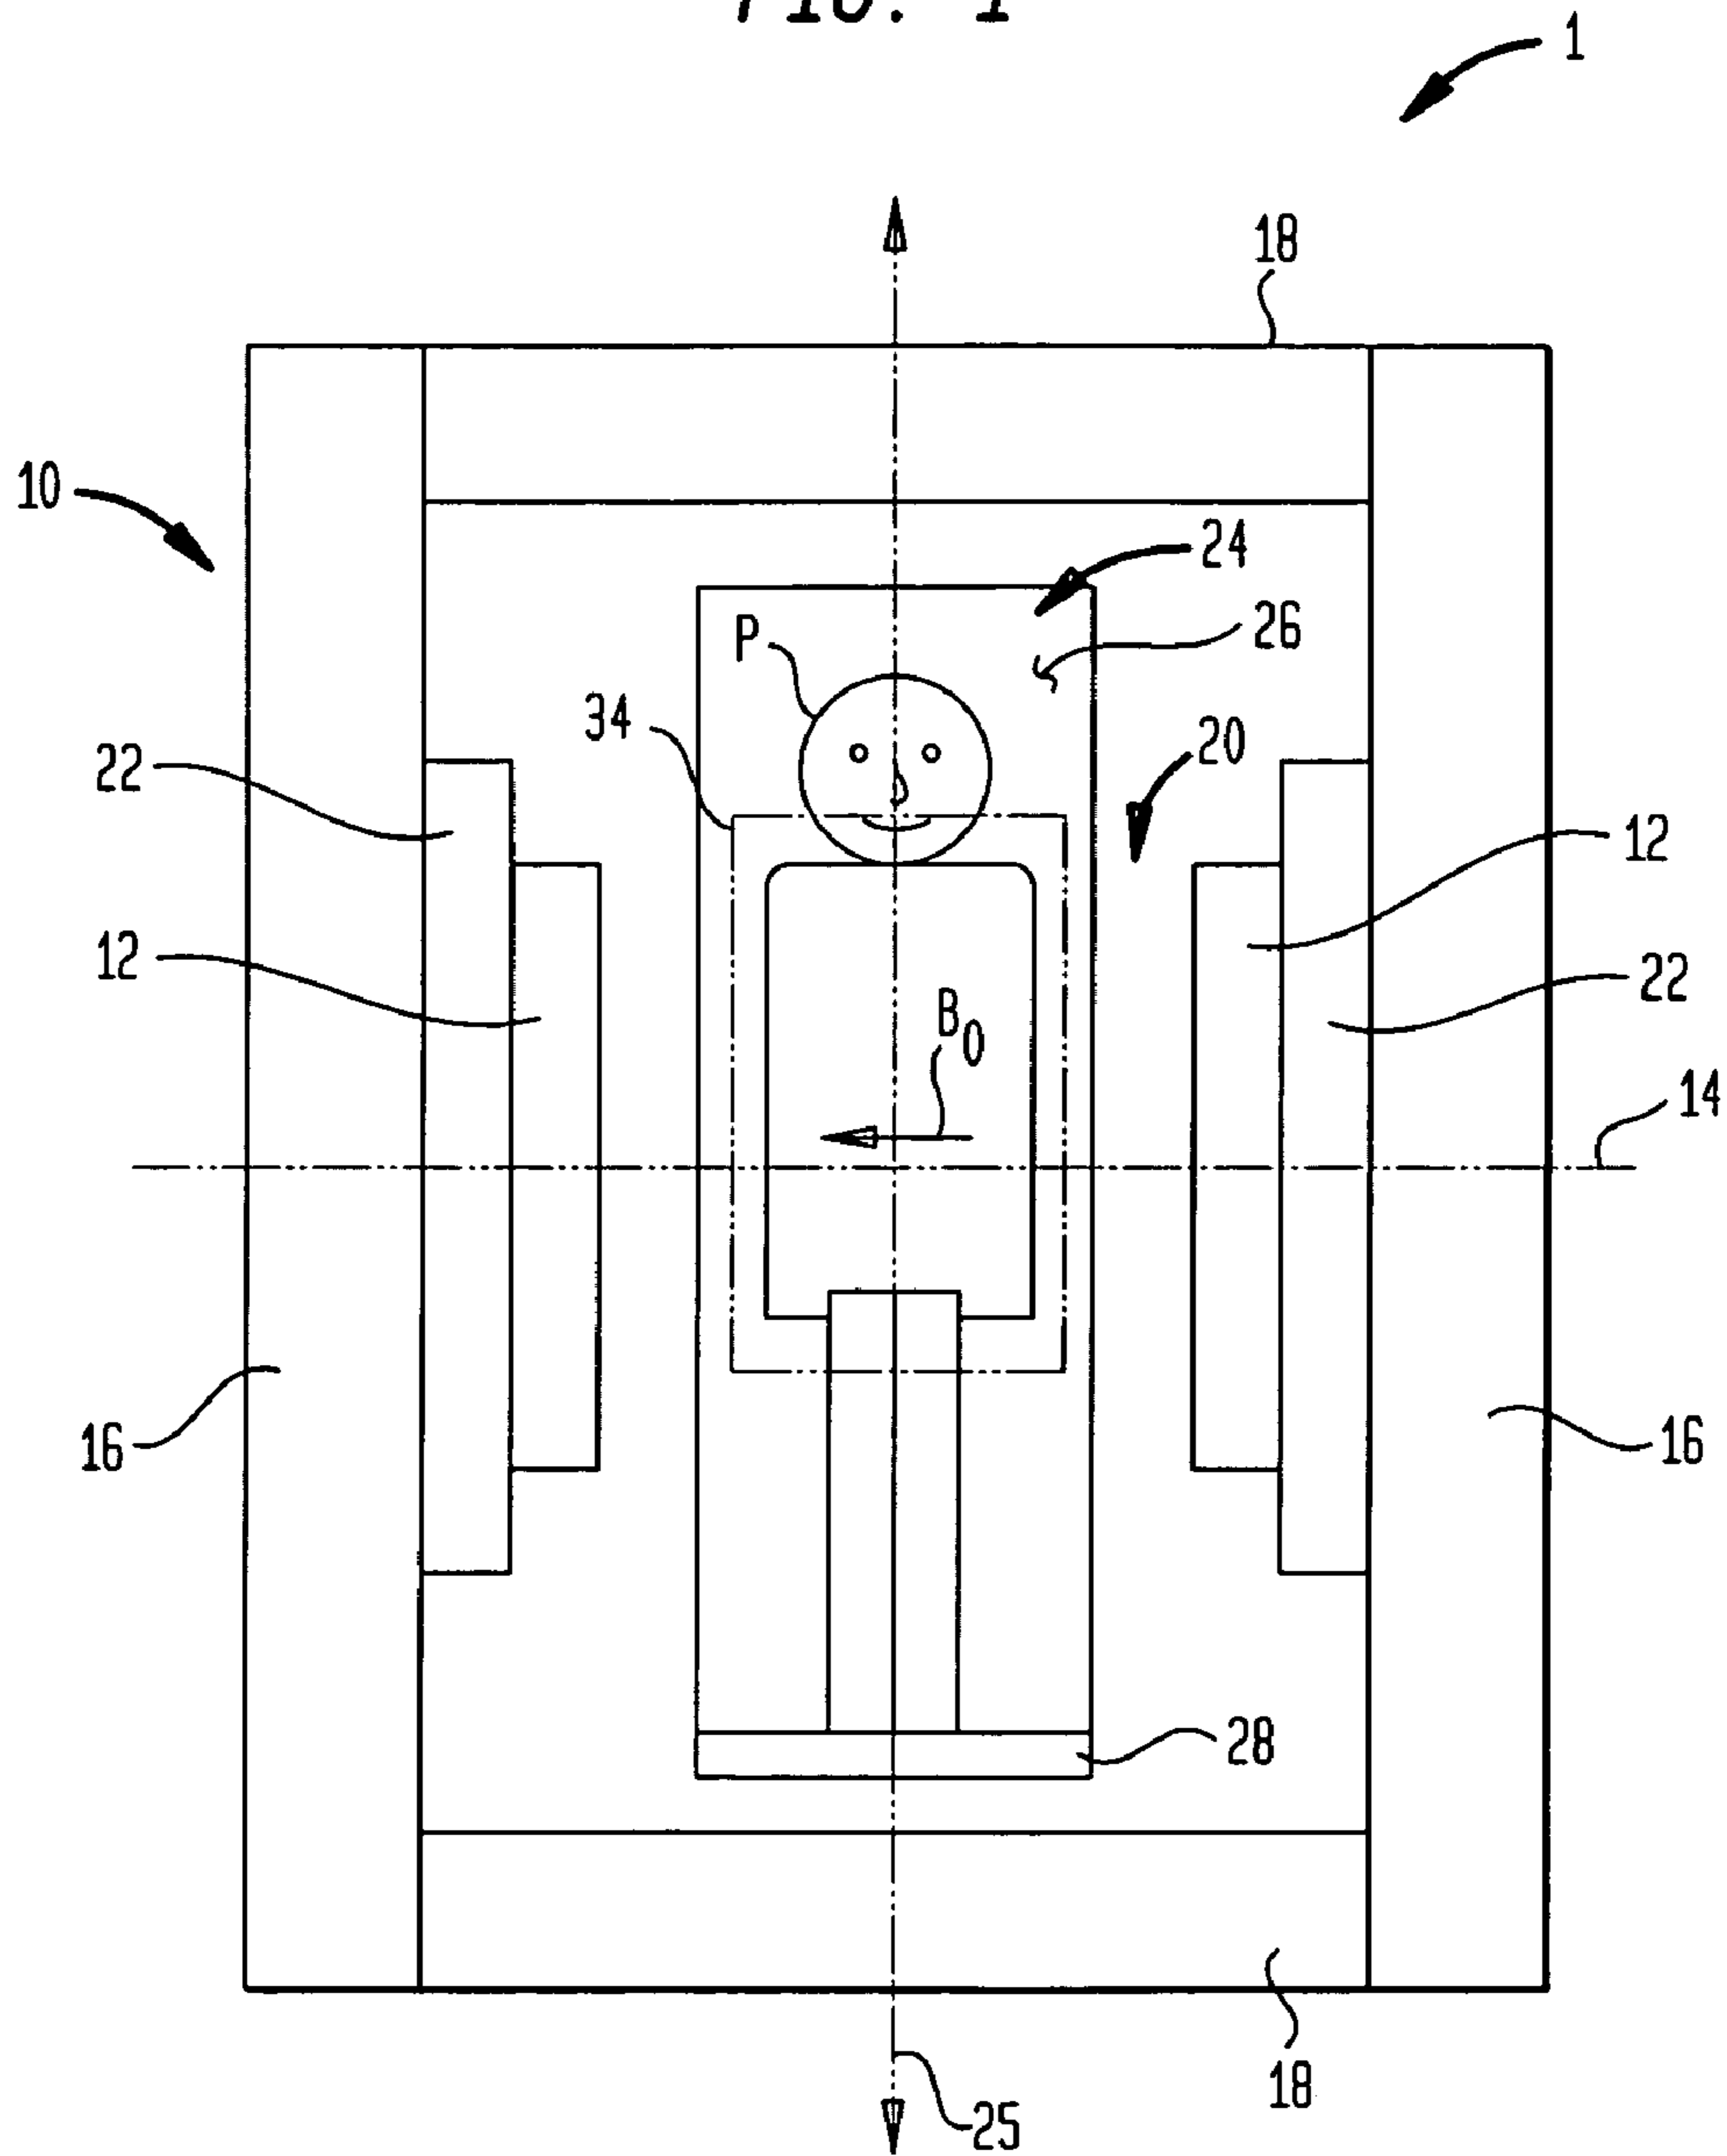


FIG. 2

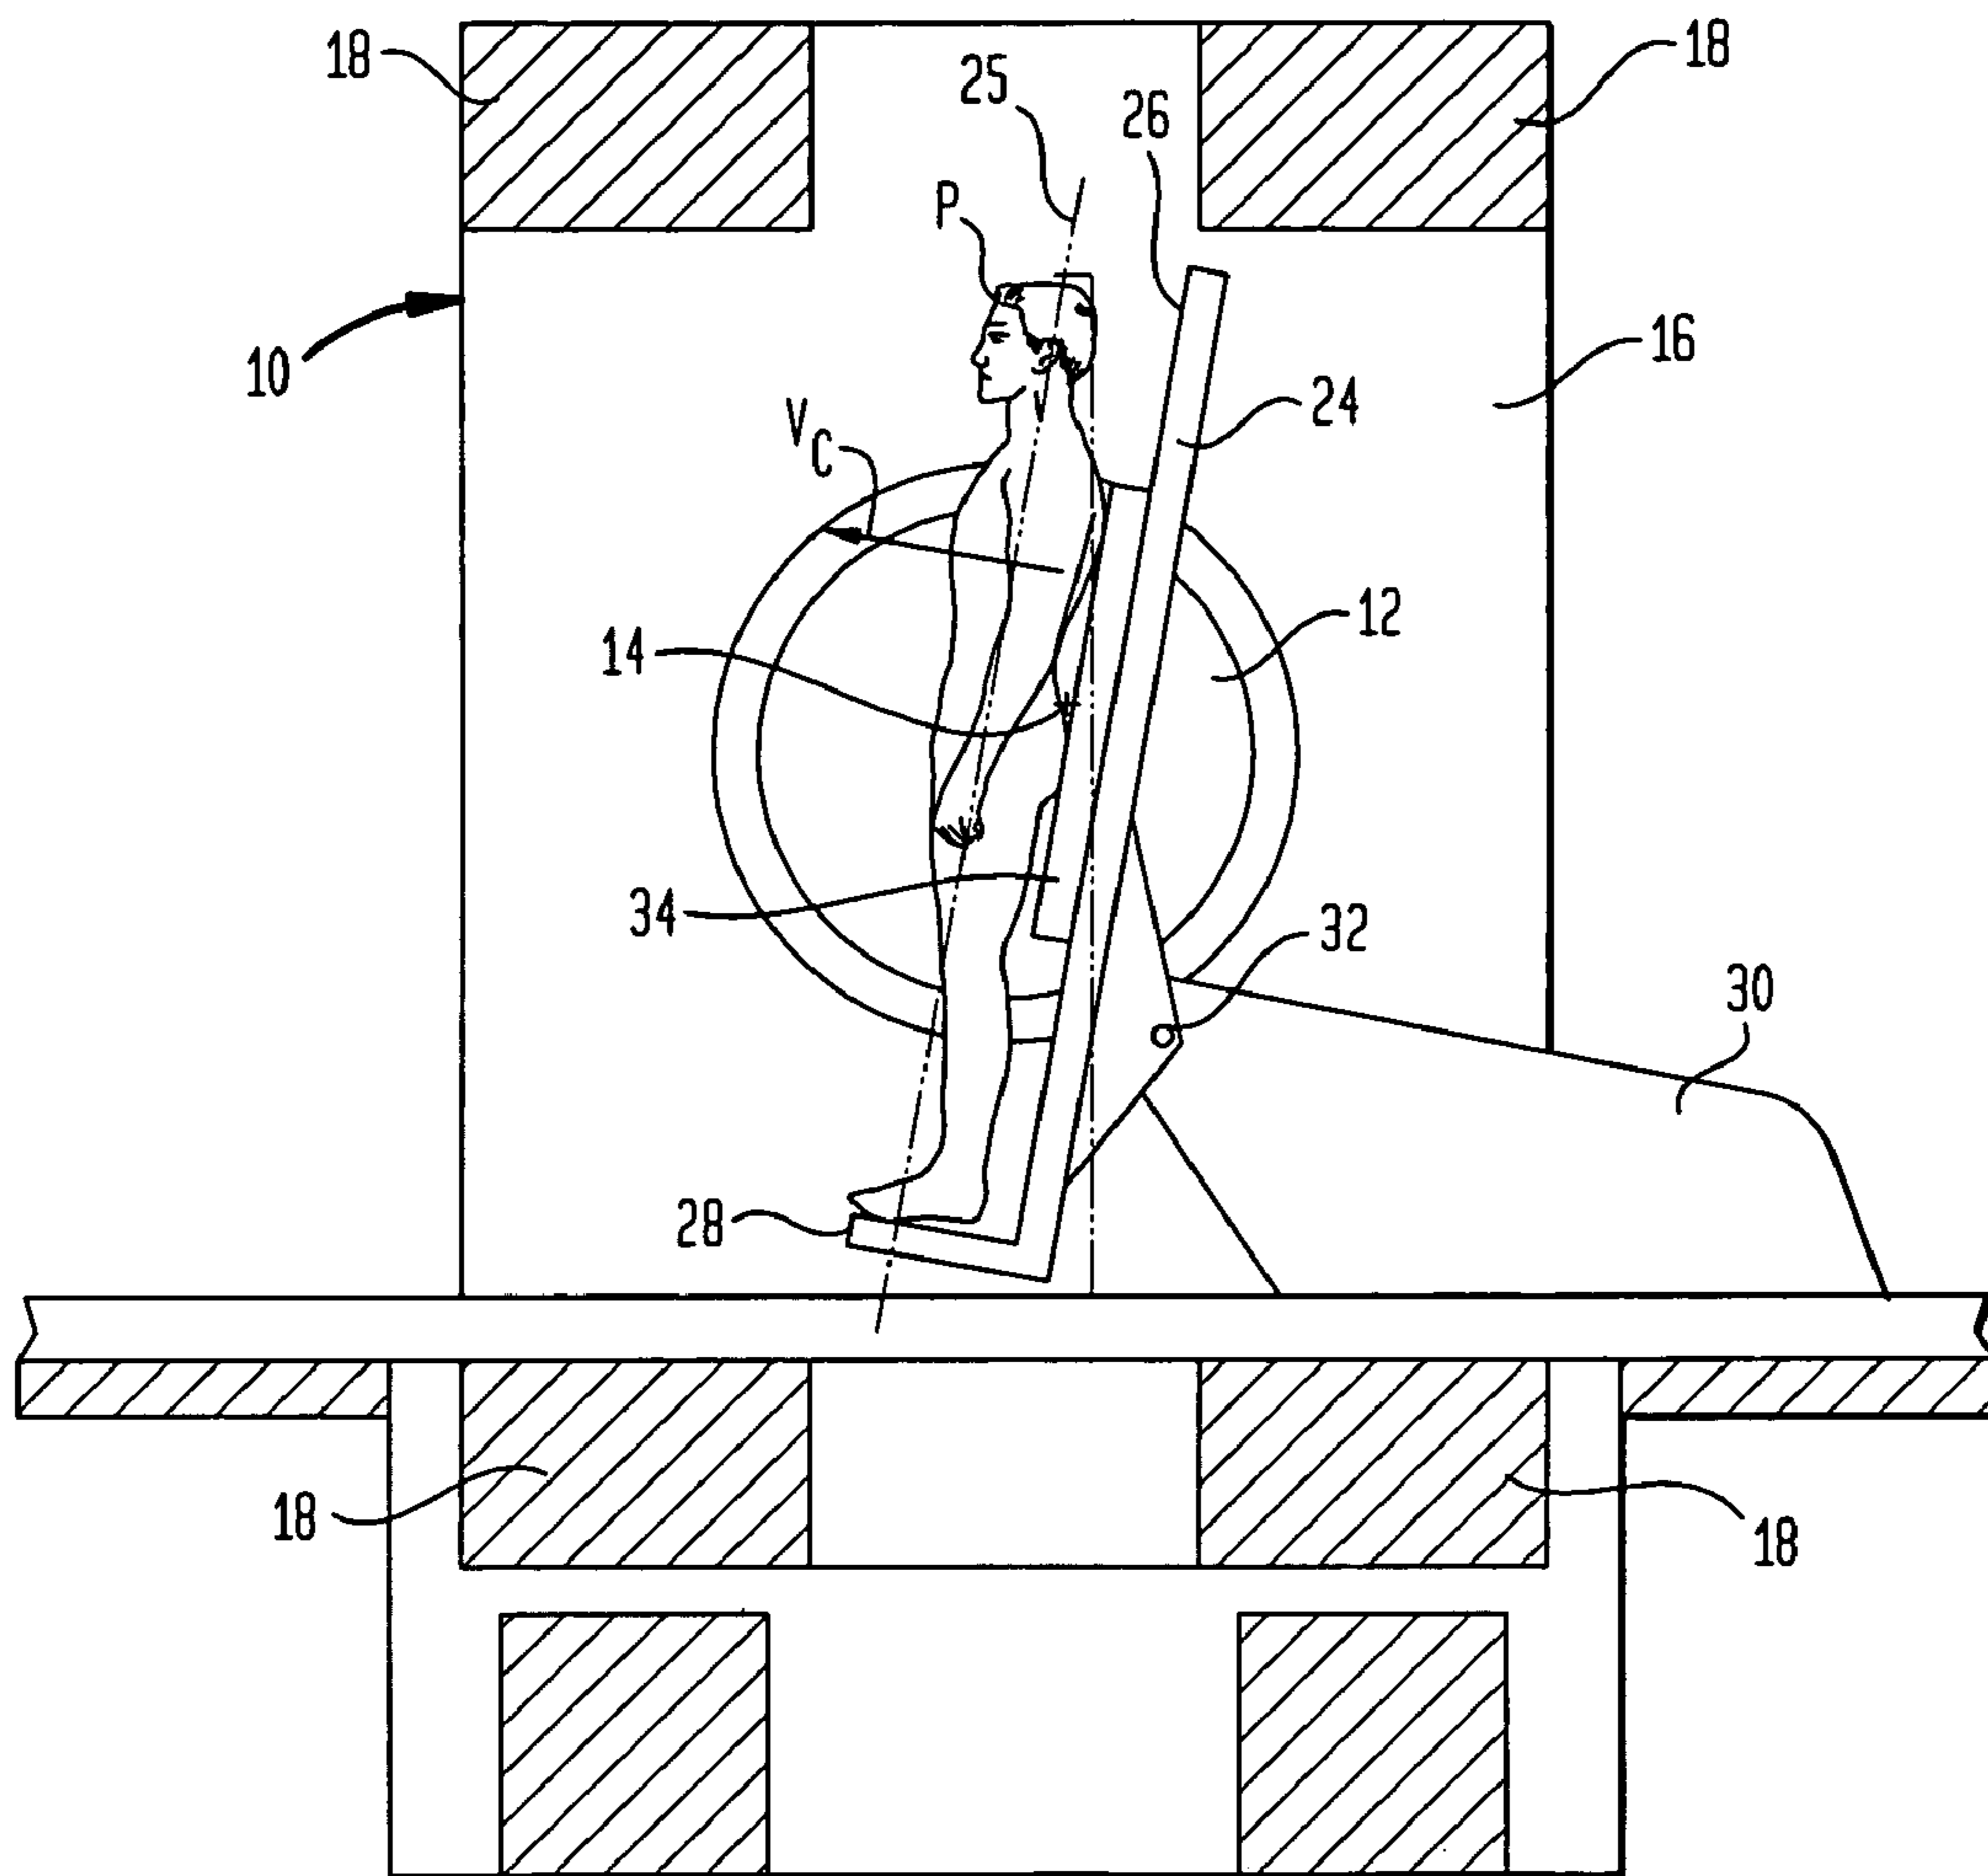


FIG. 3

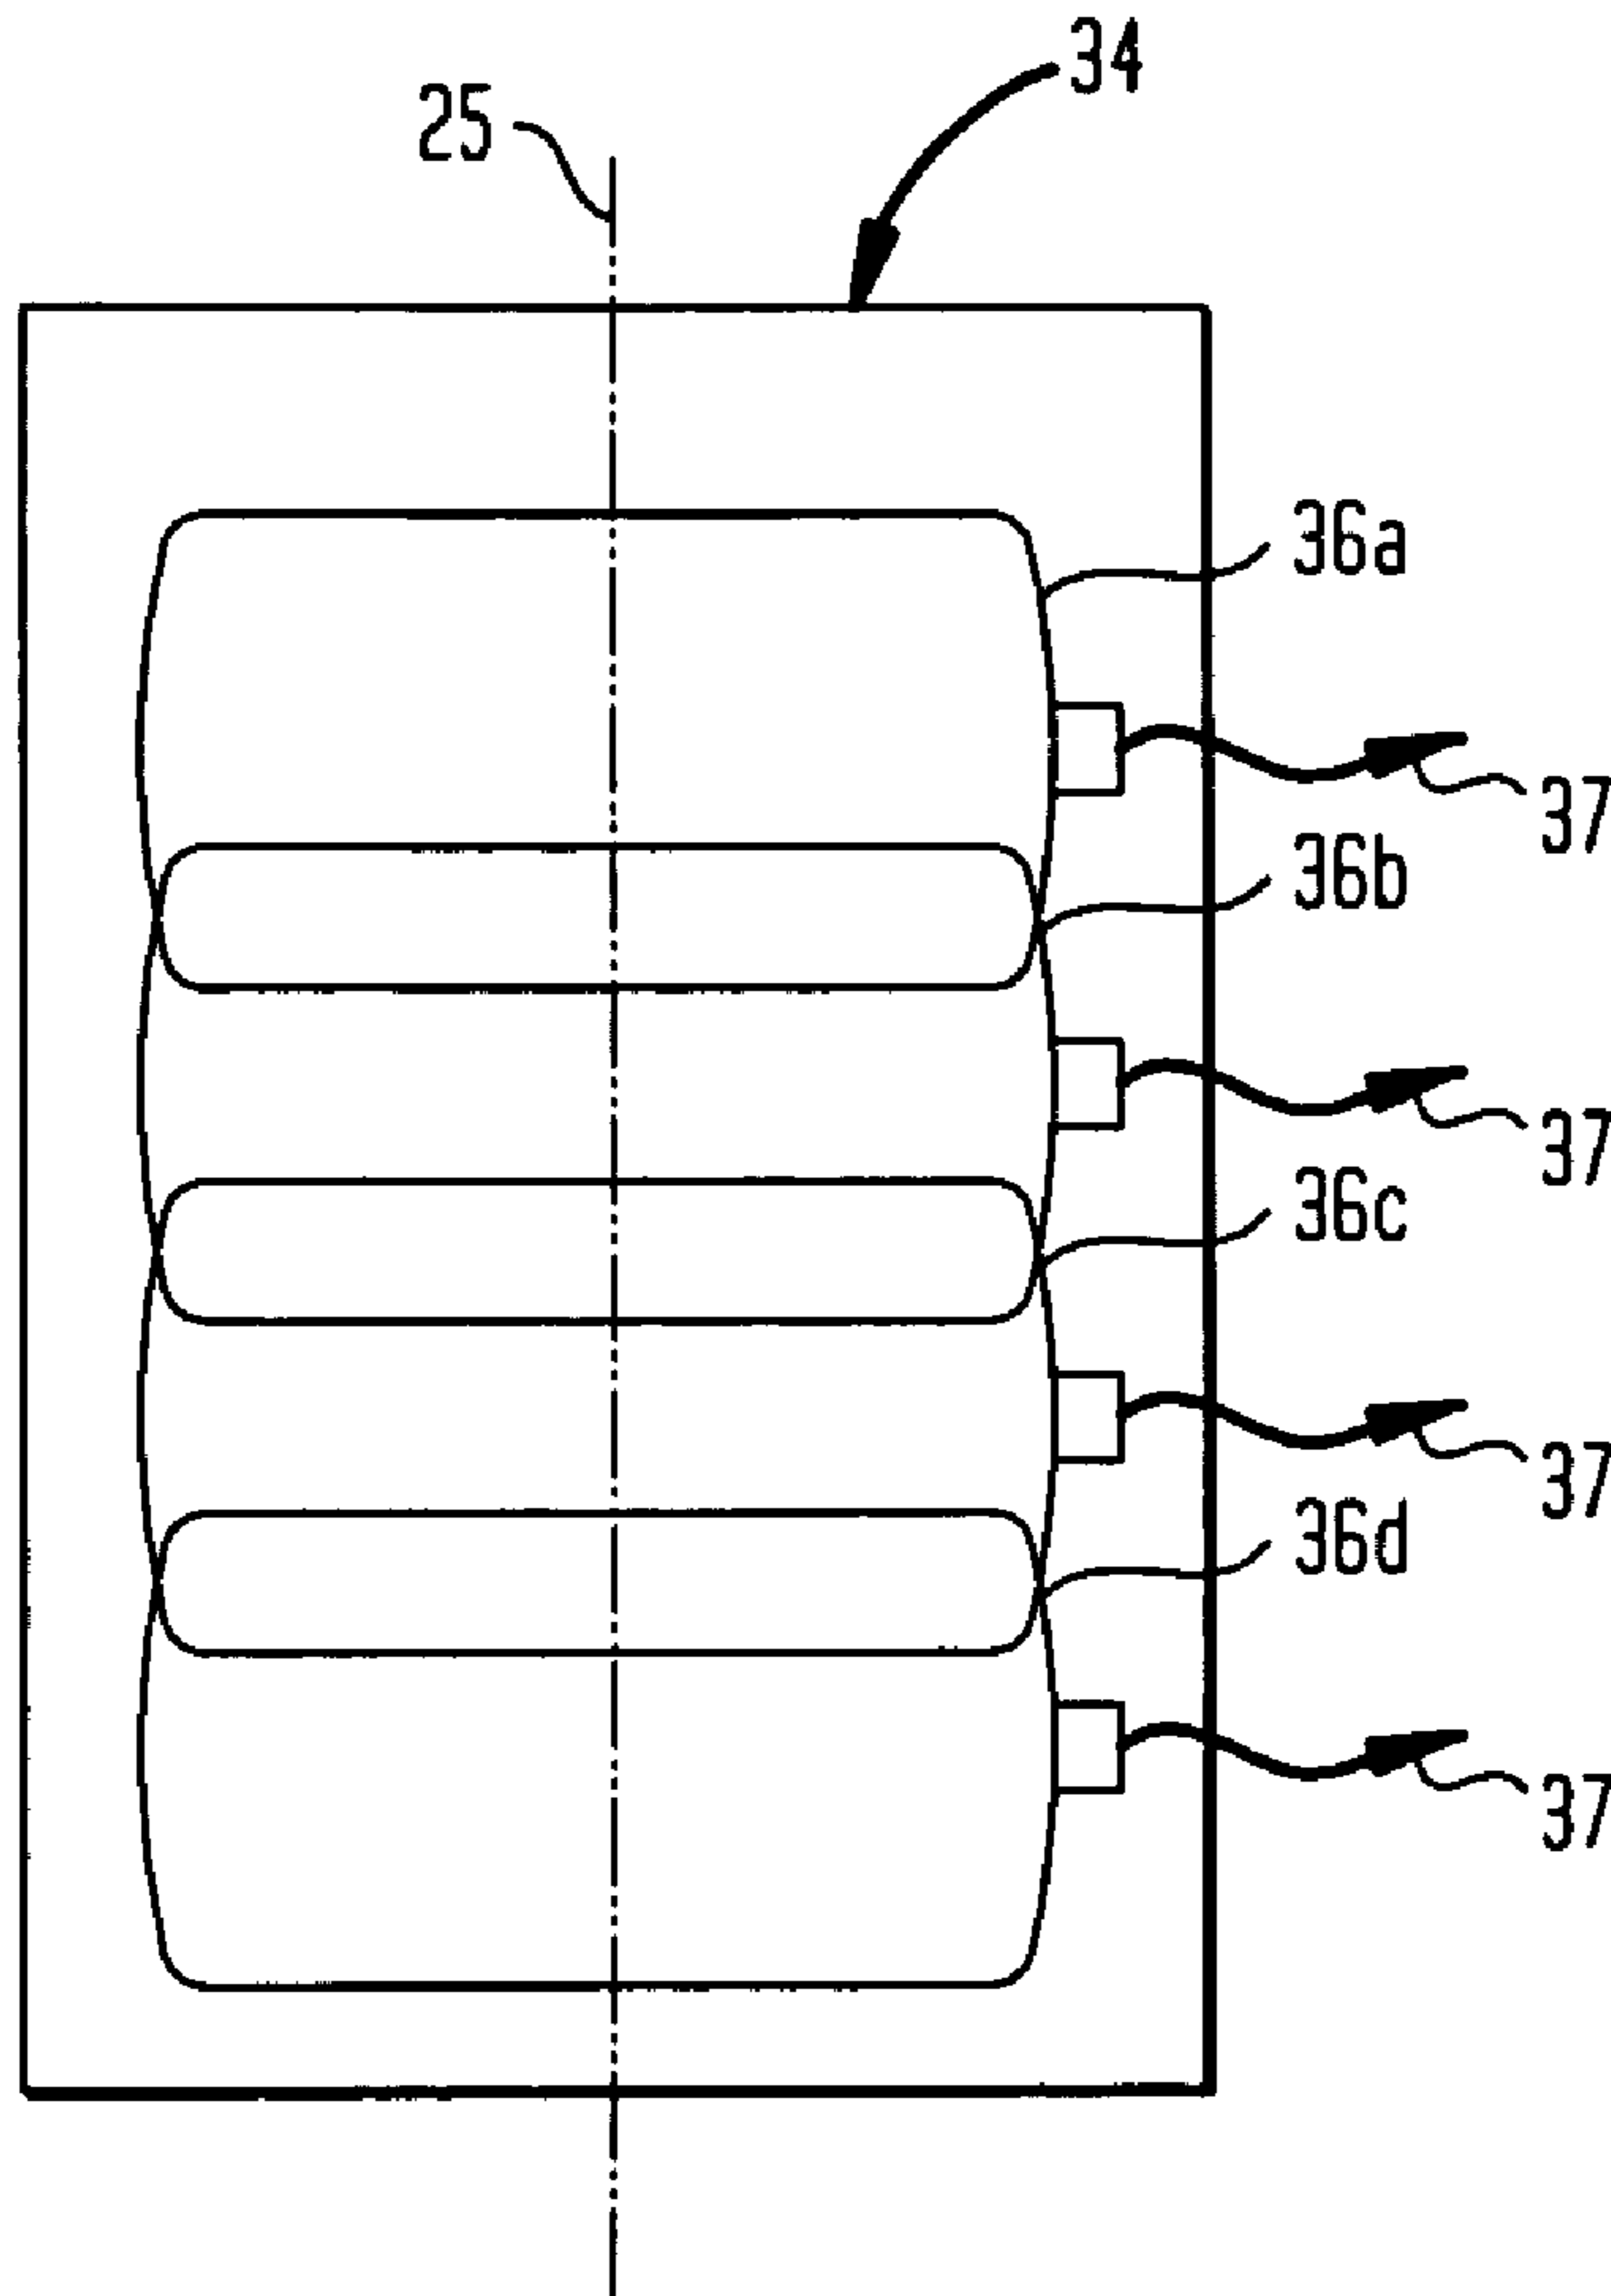


FIG. 4

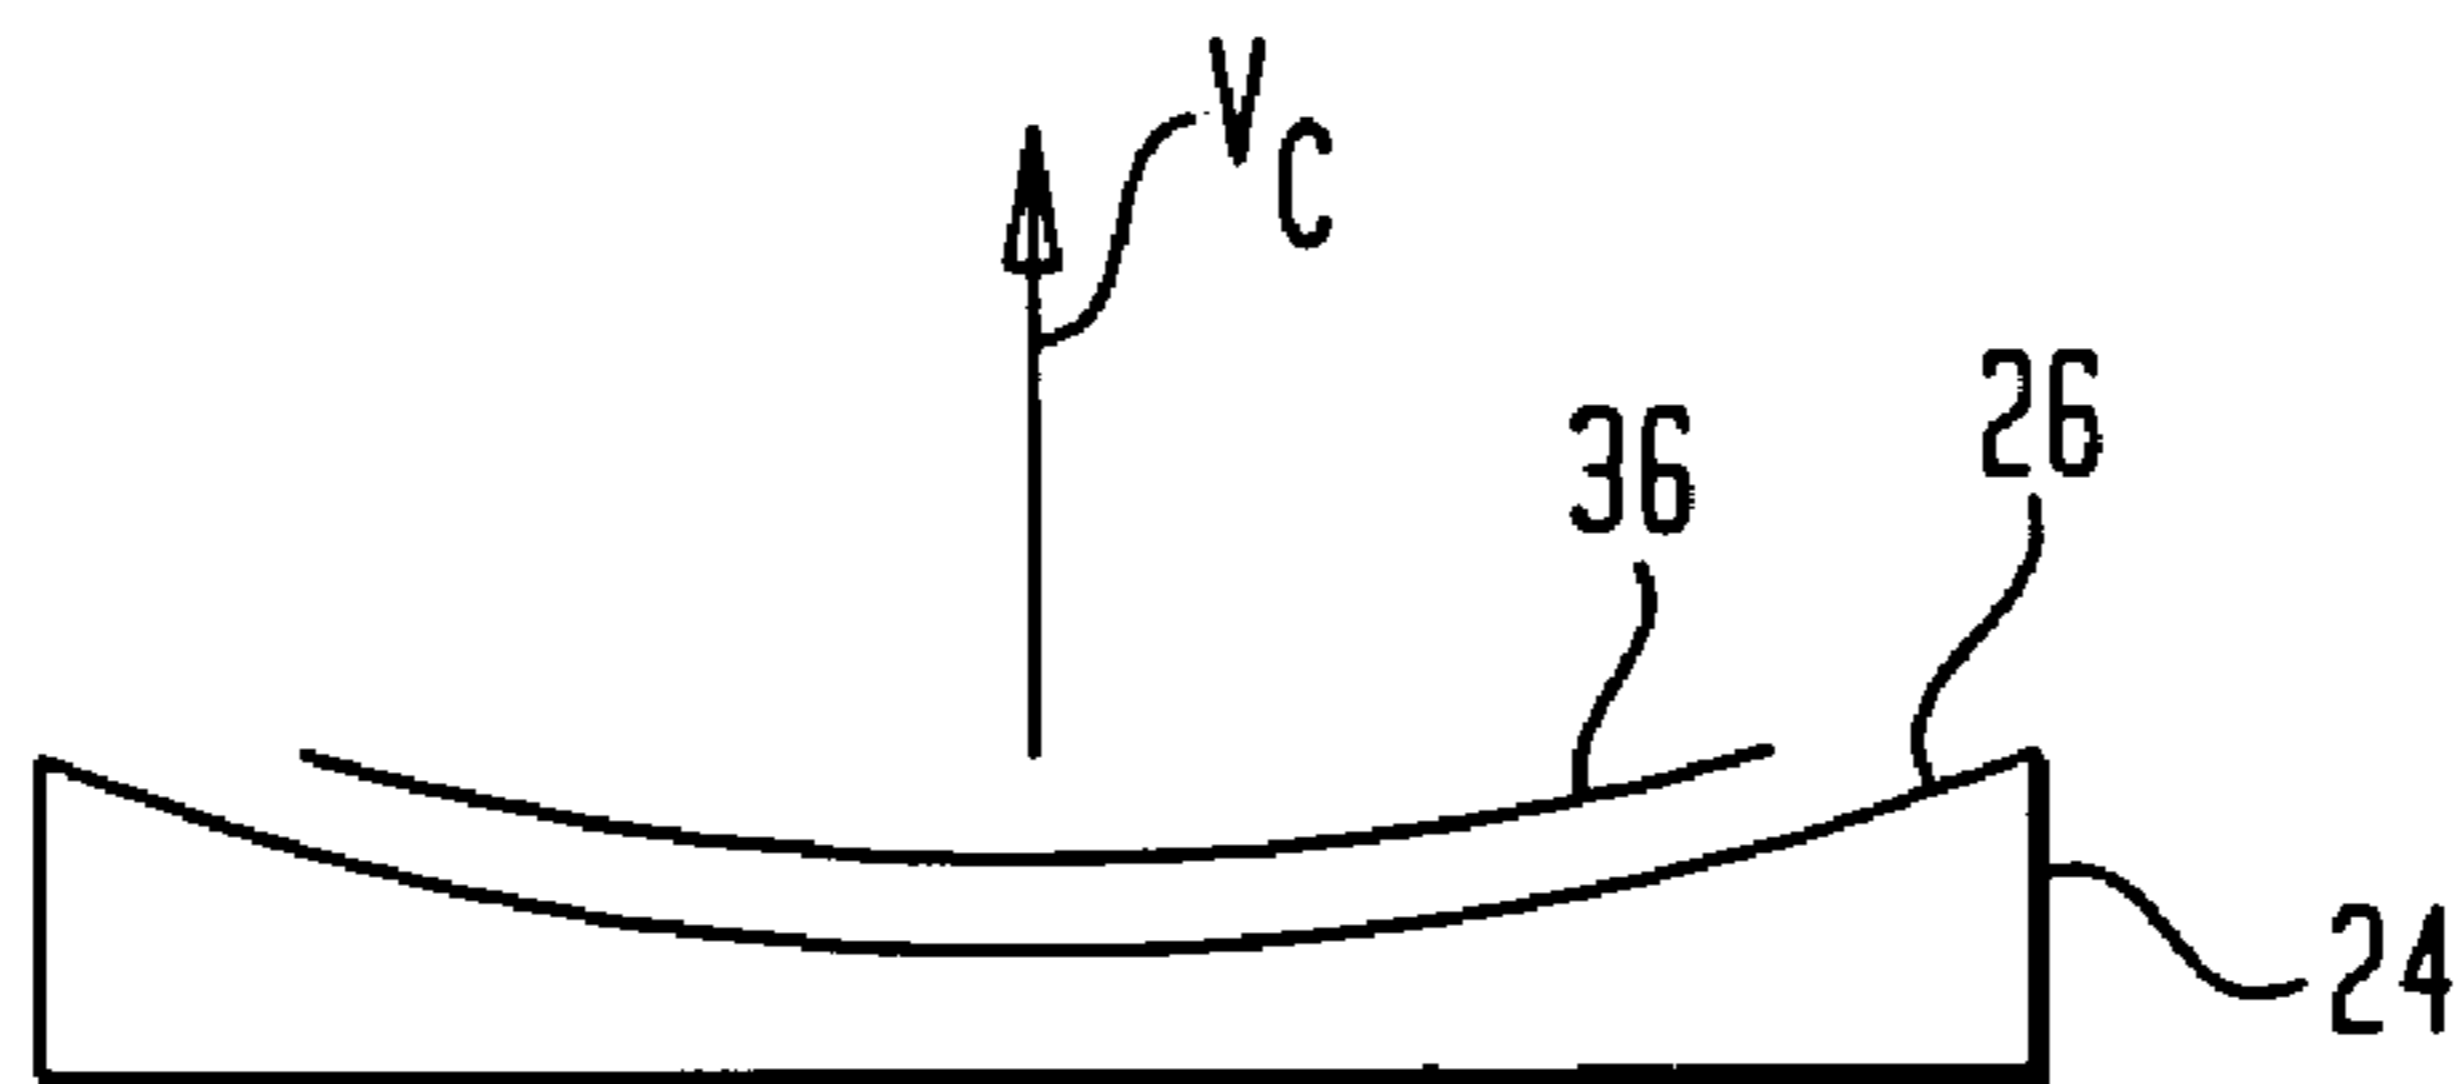
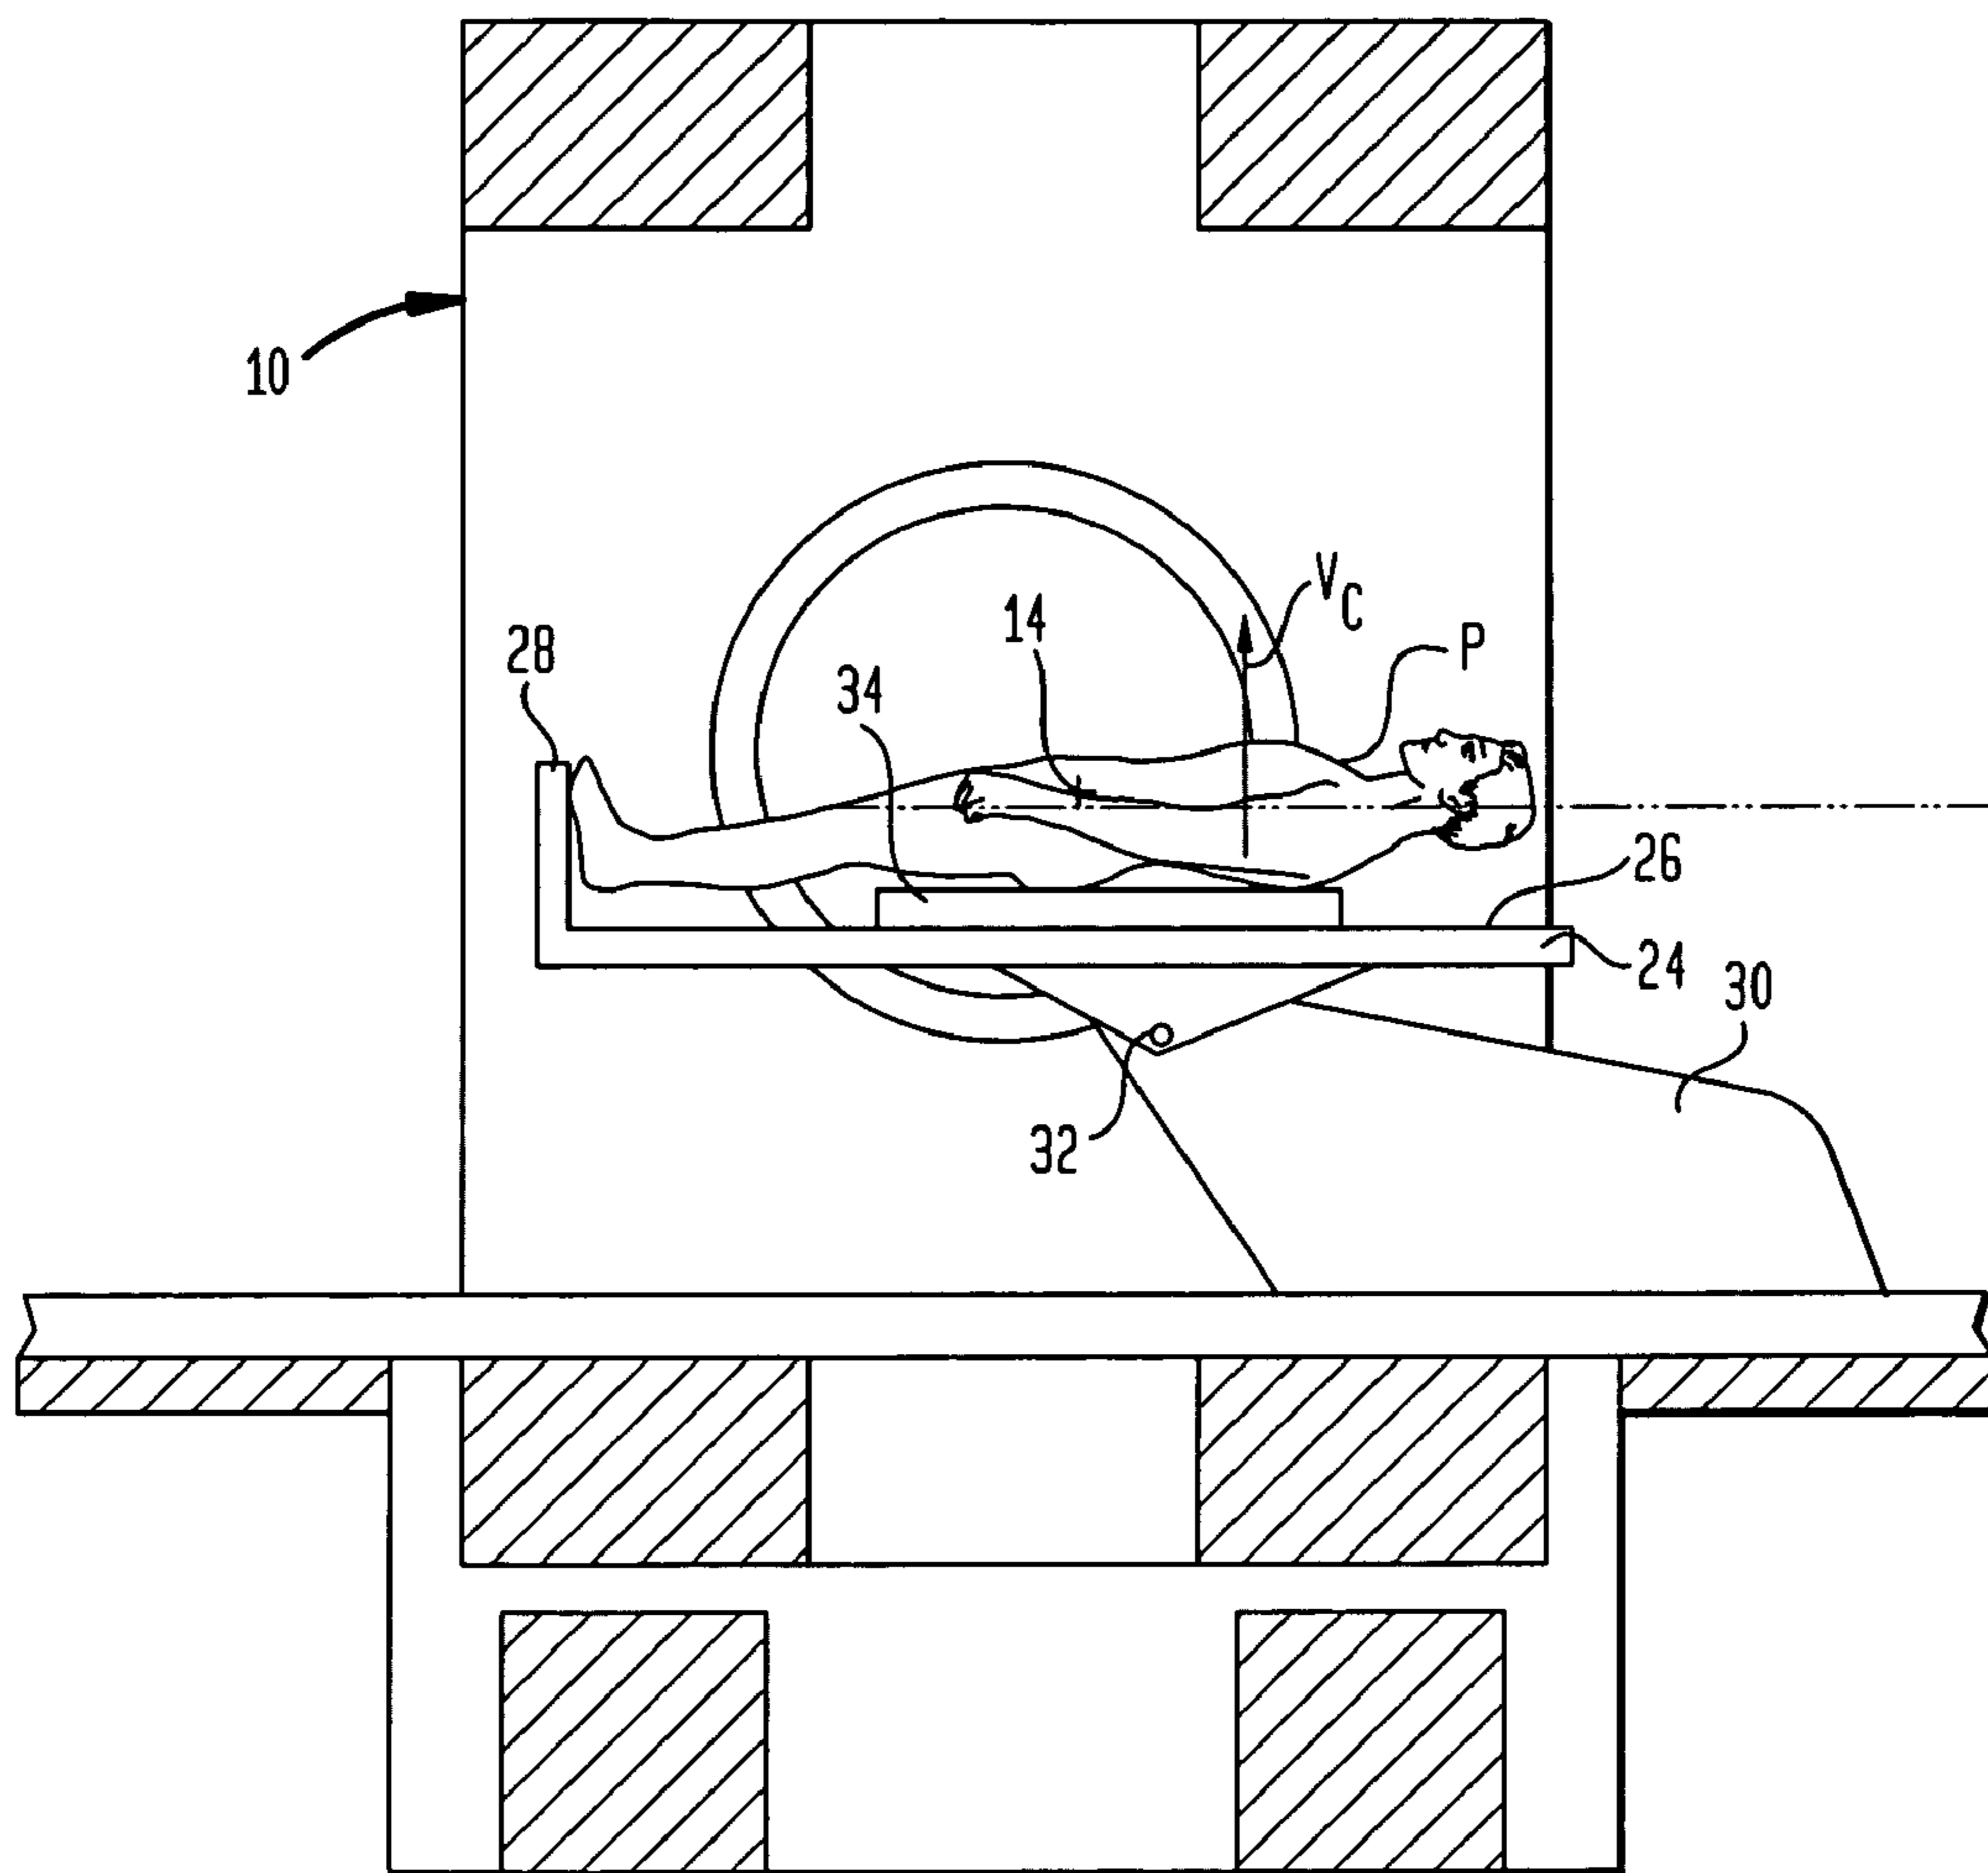


FIG. 5



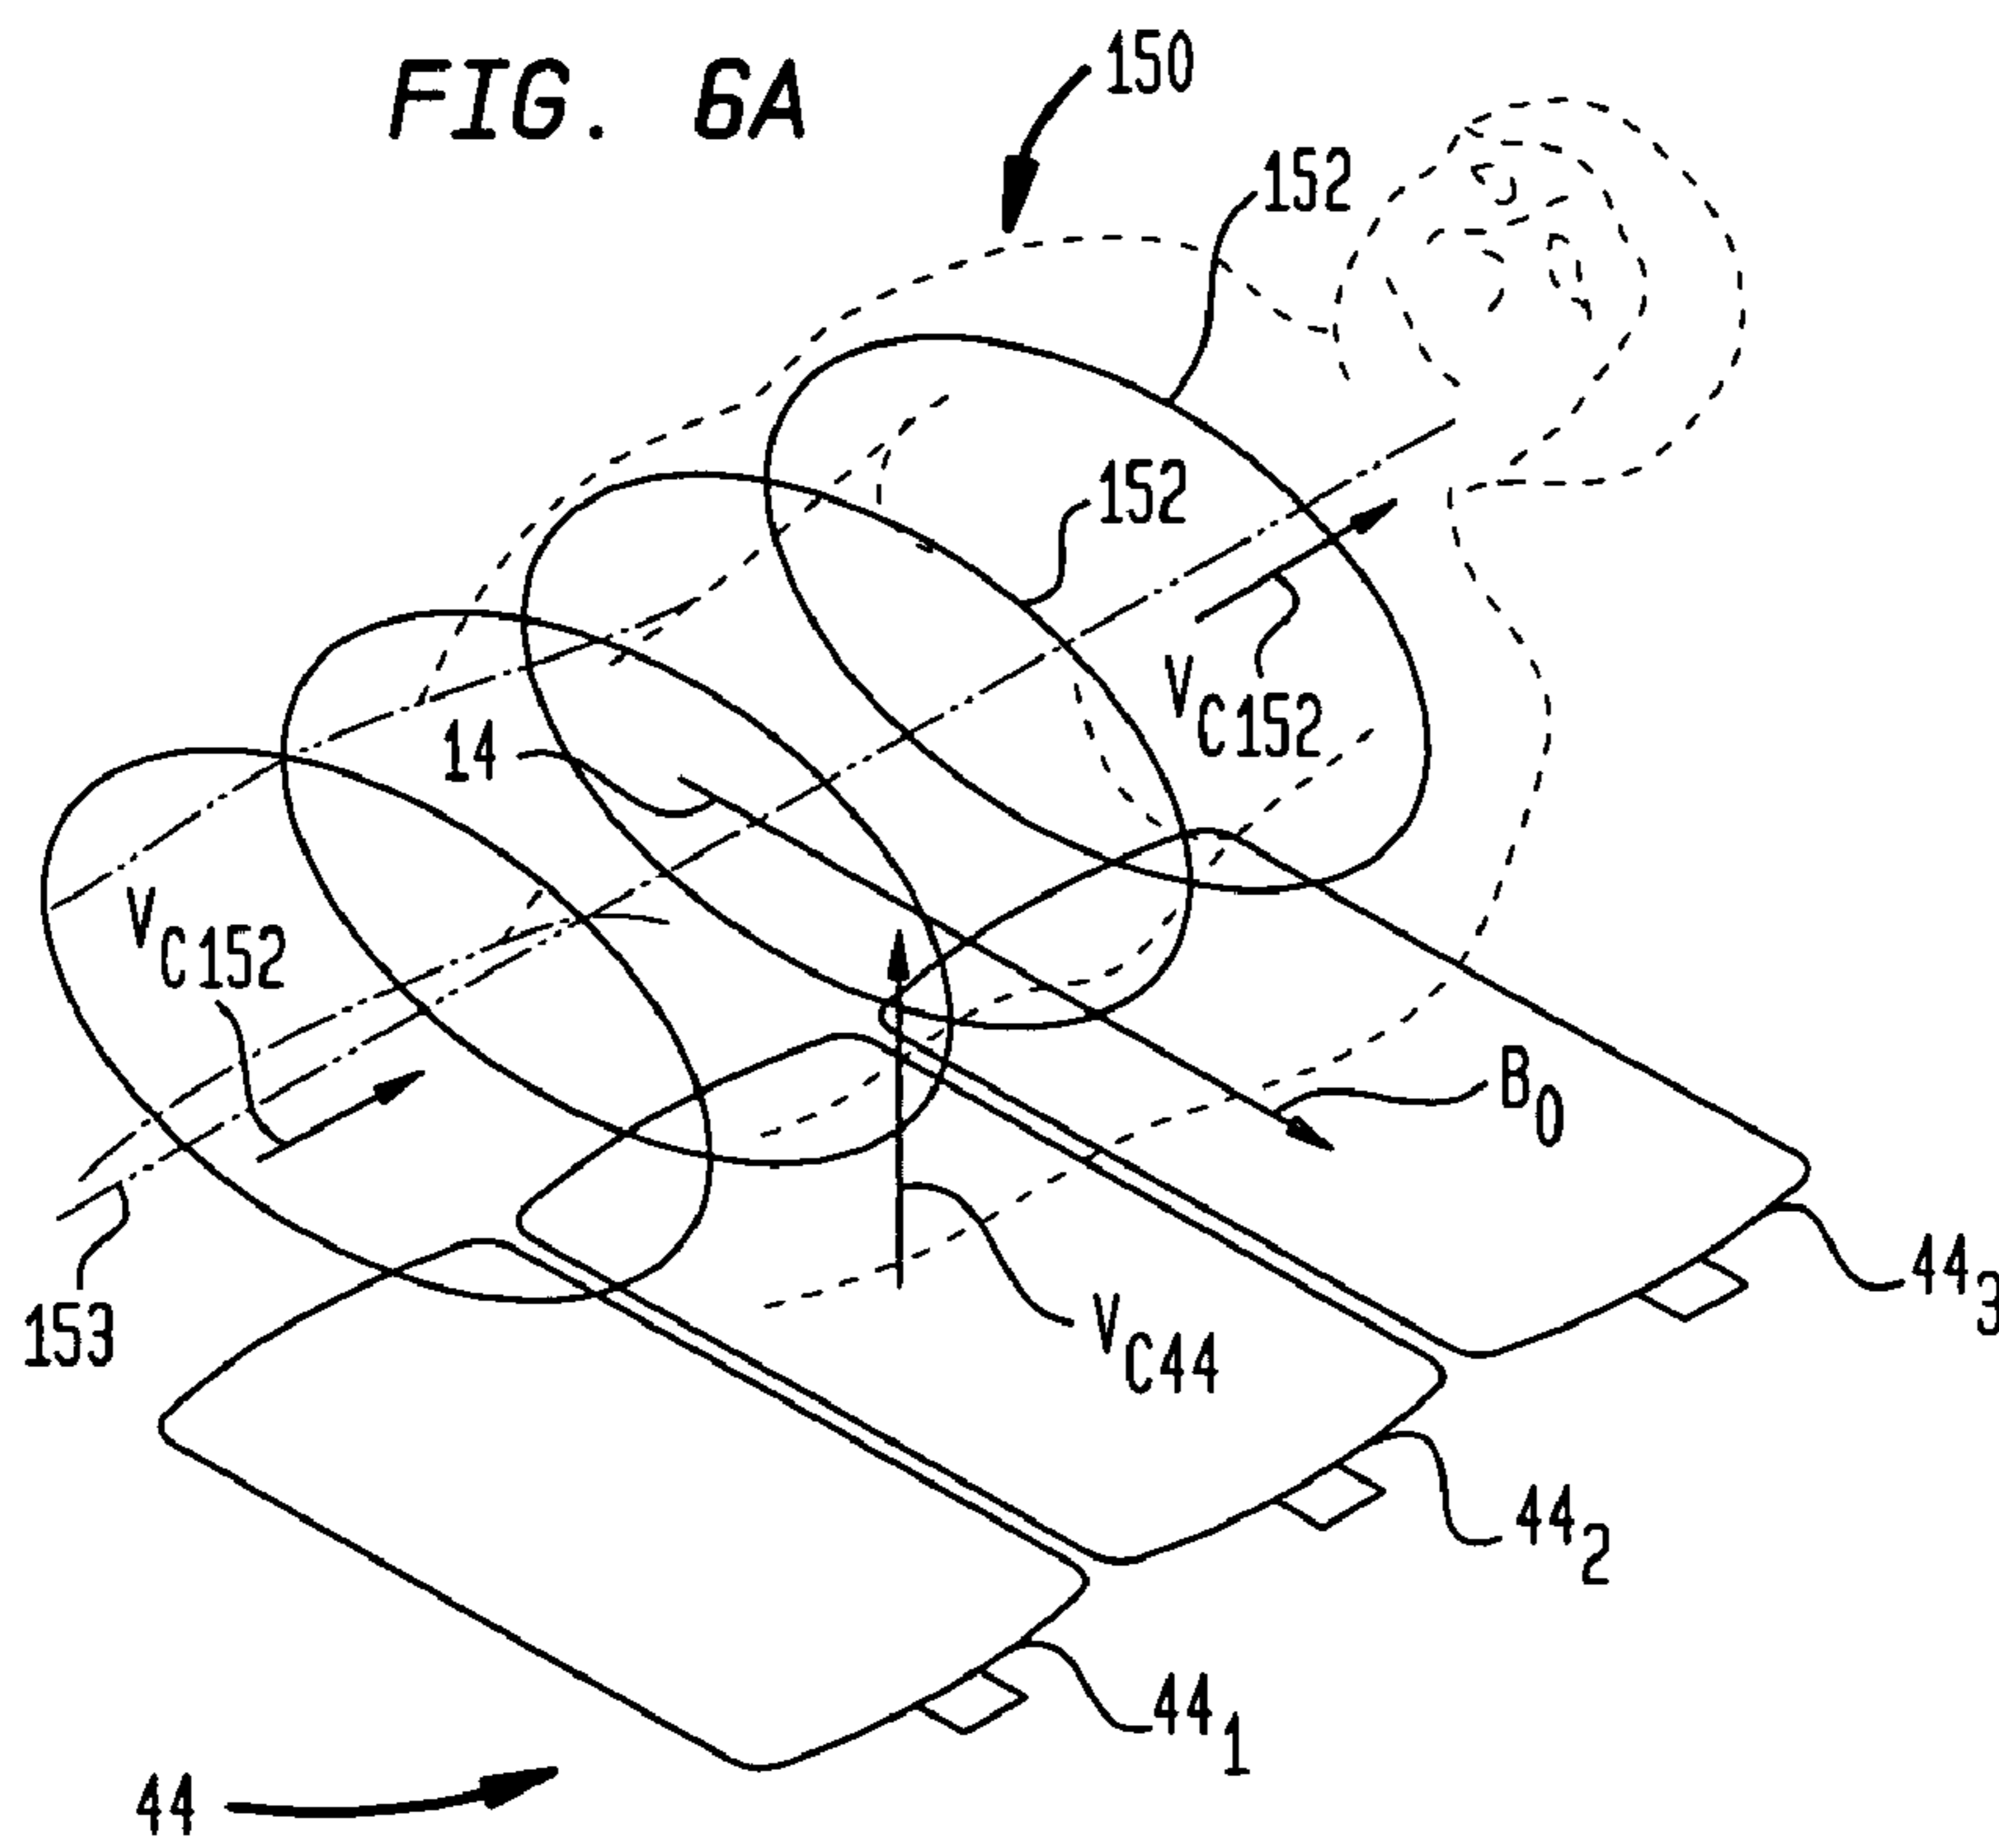
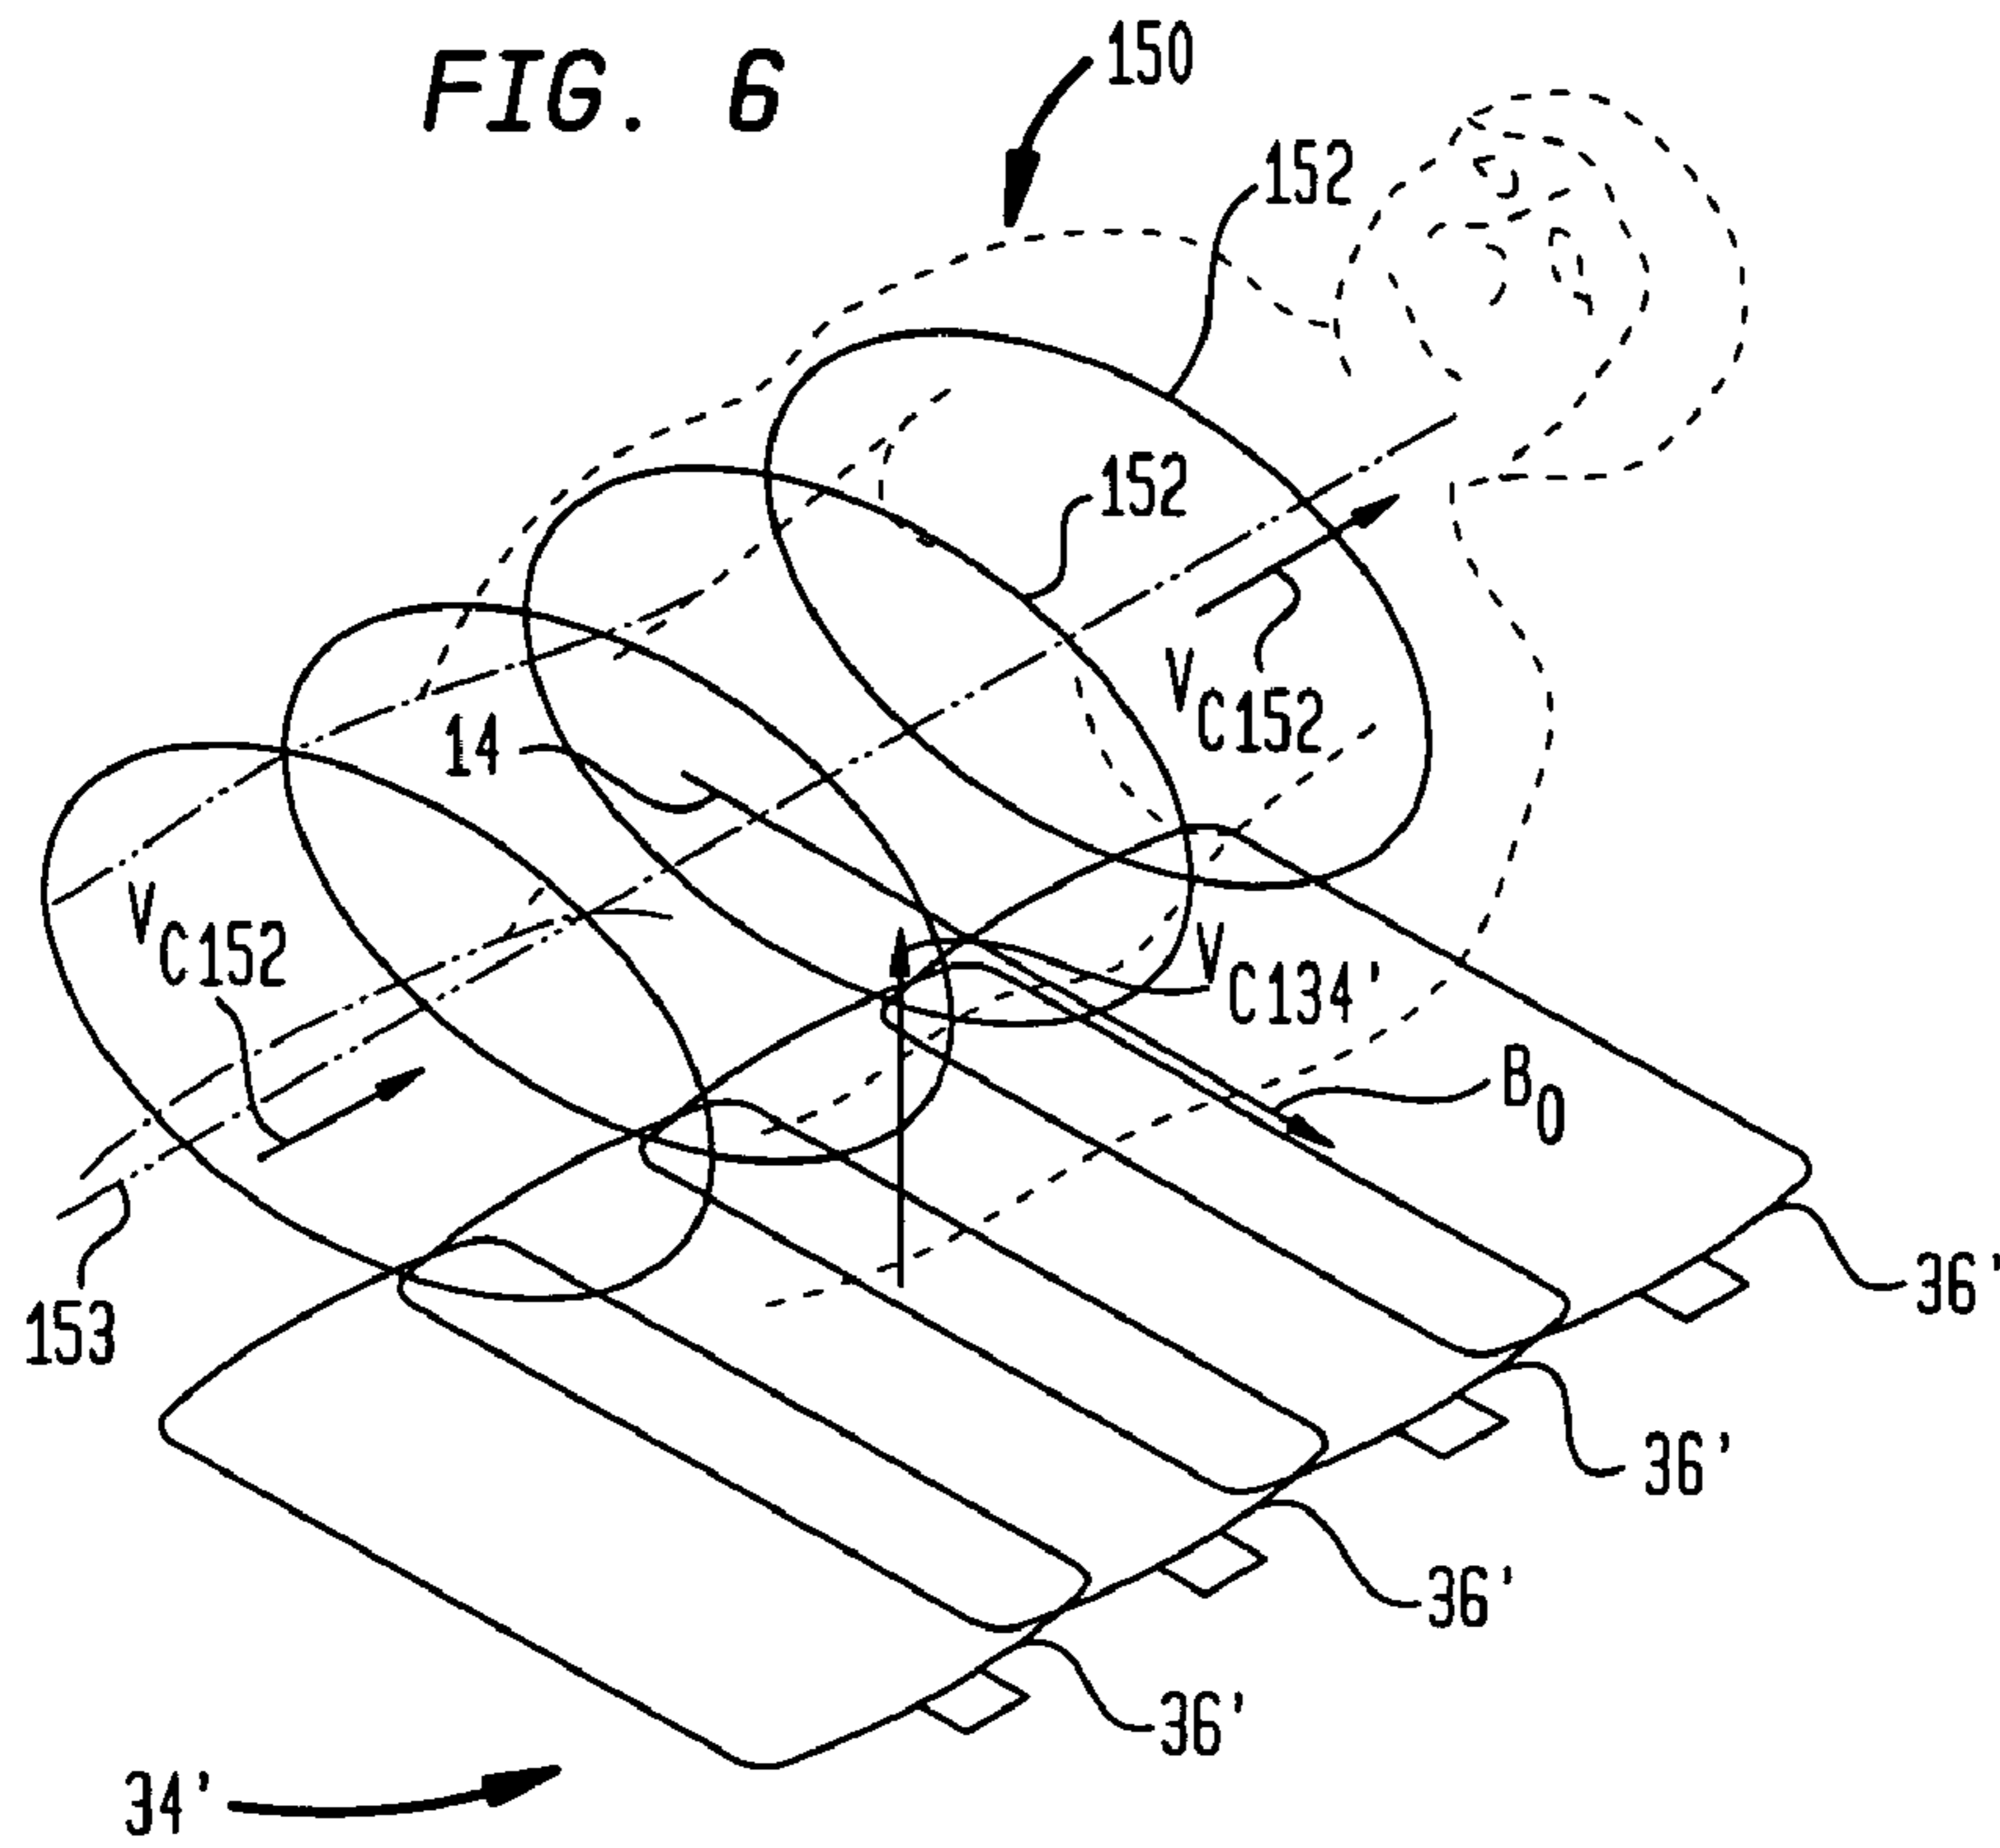




FIG. 7

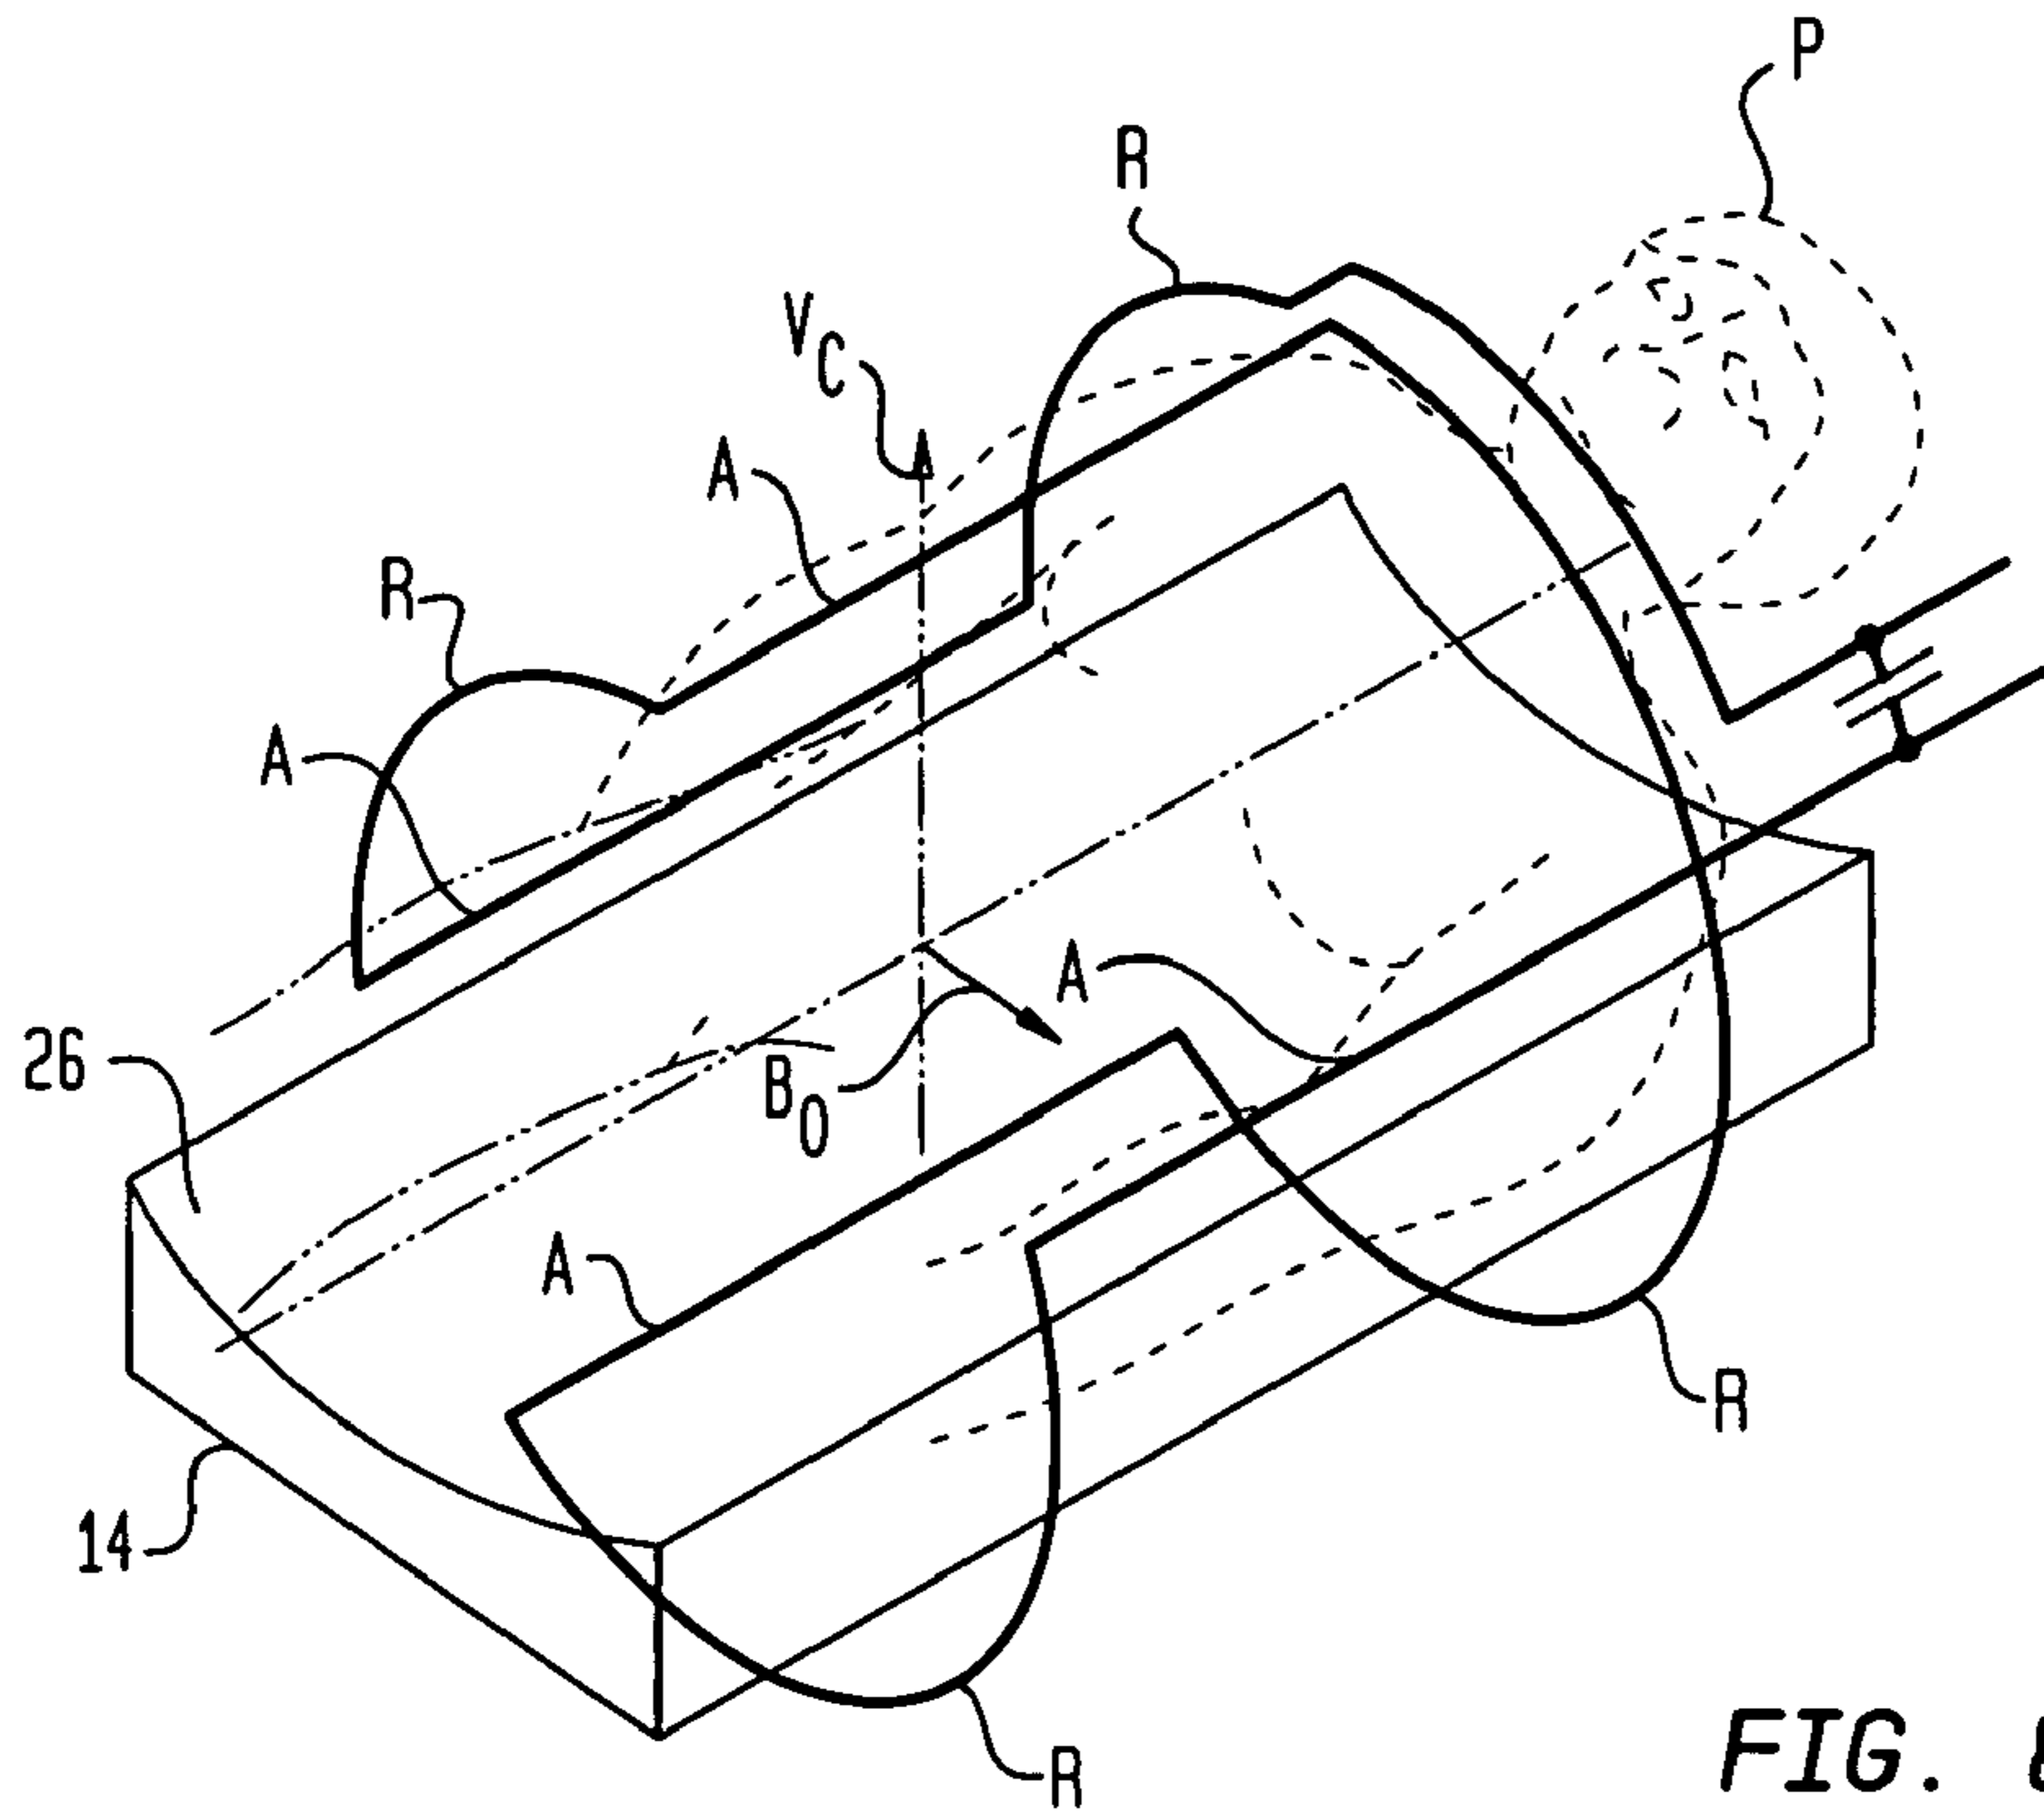
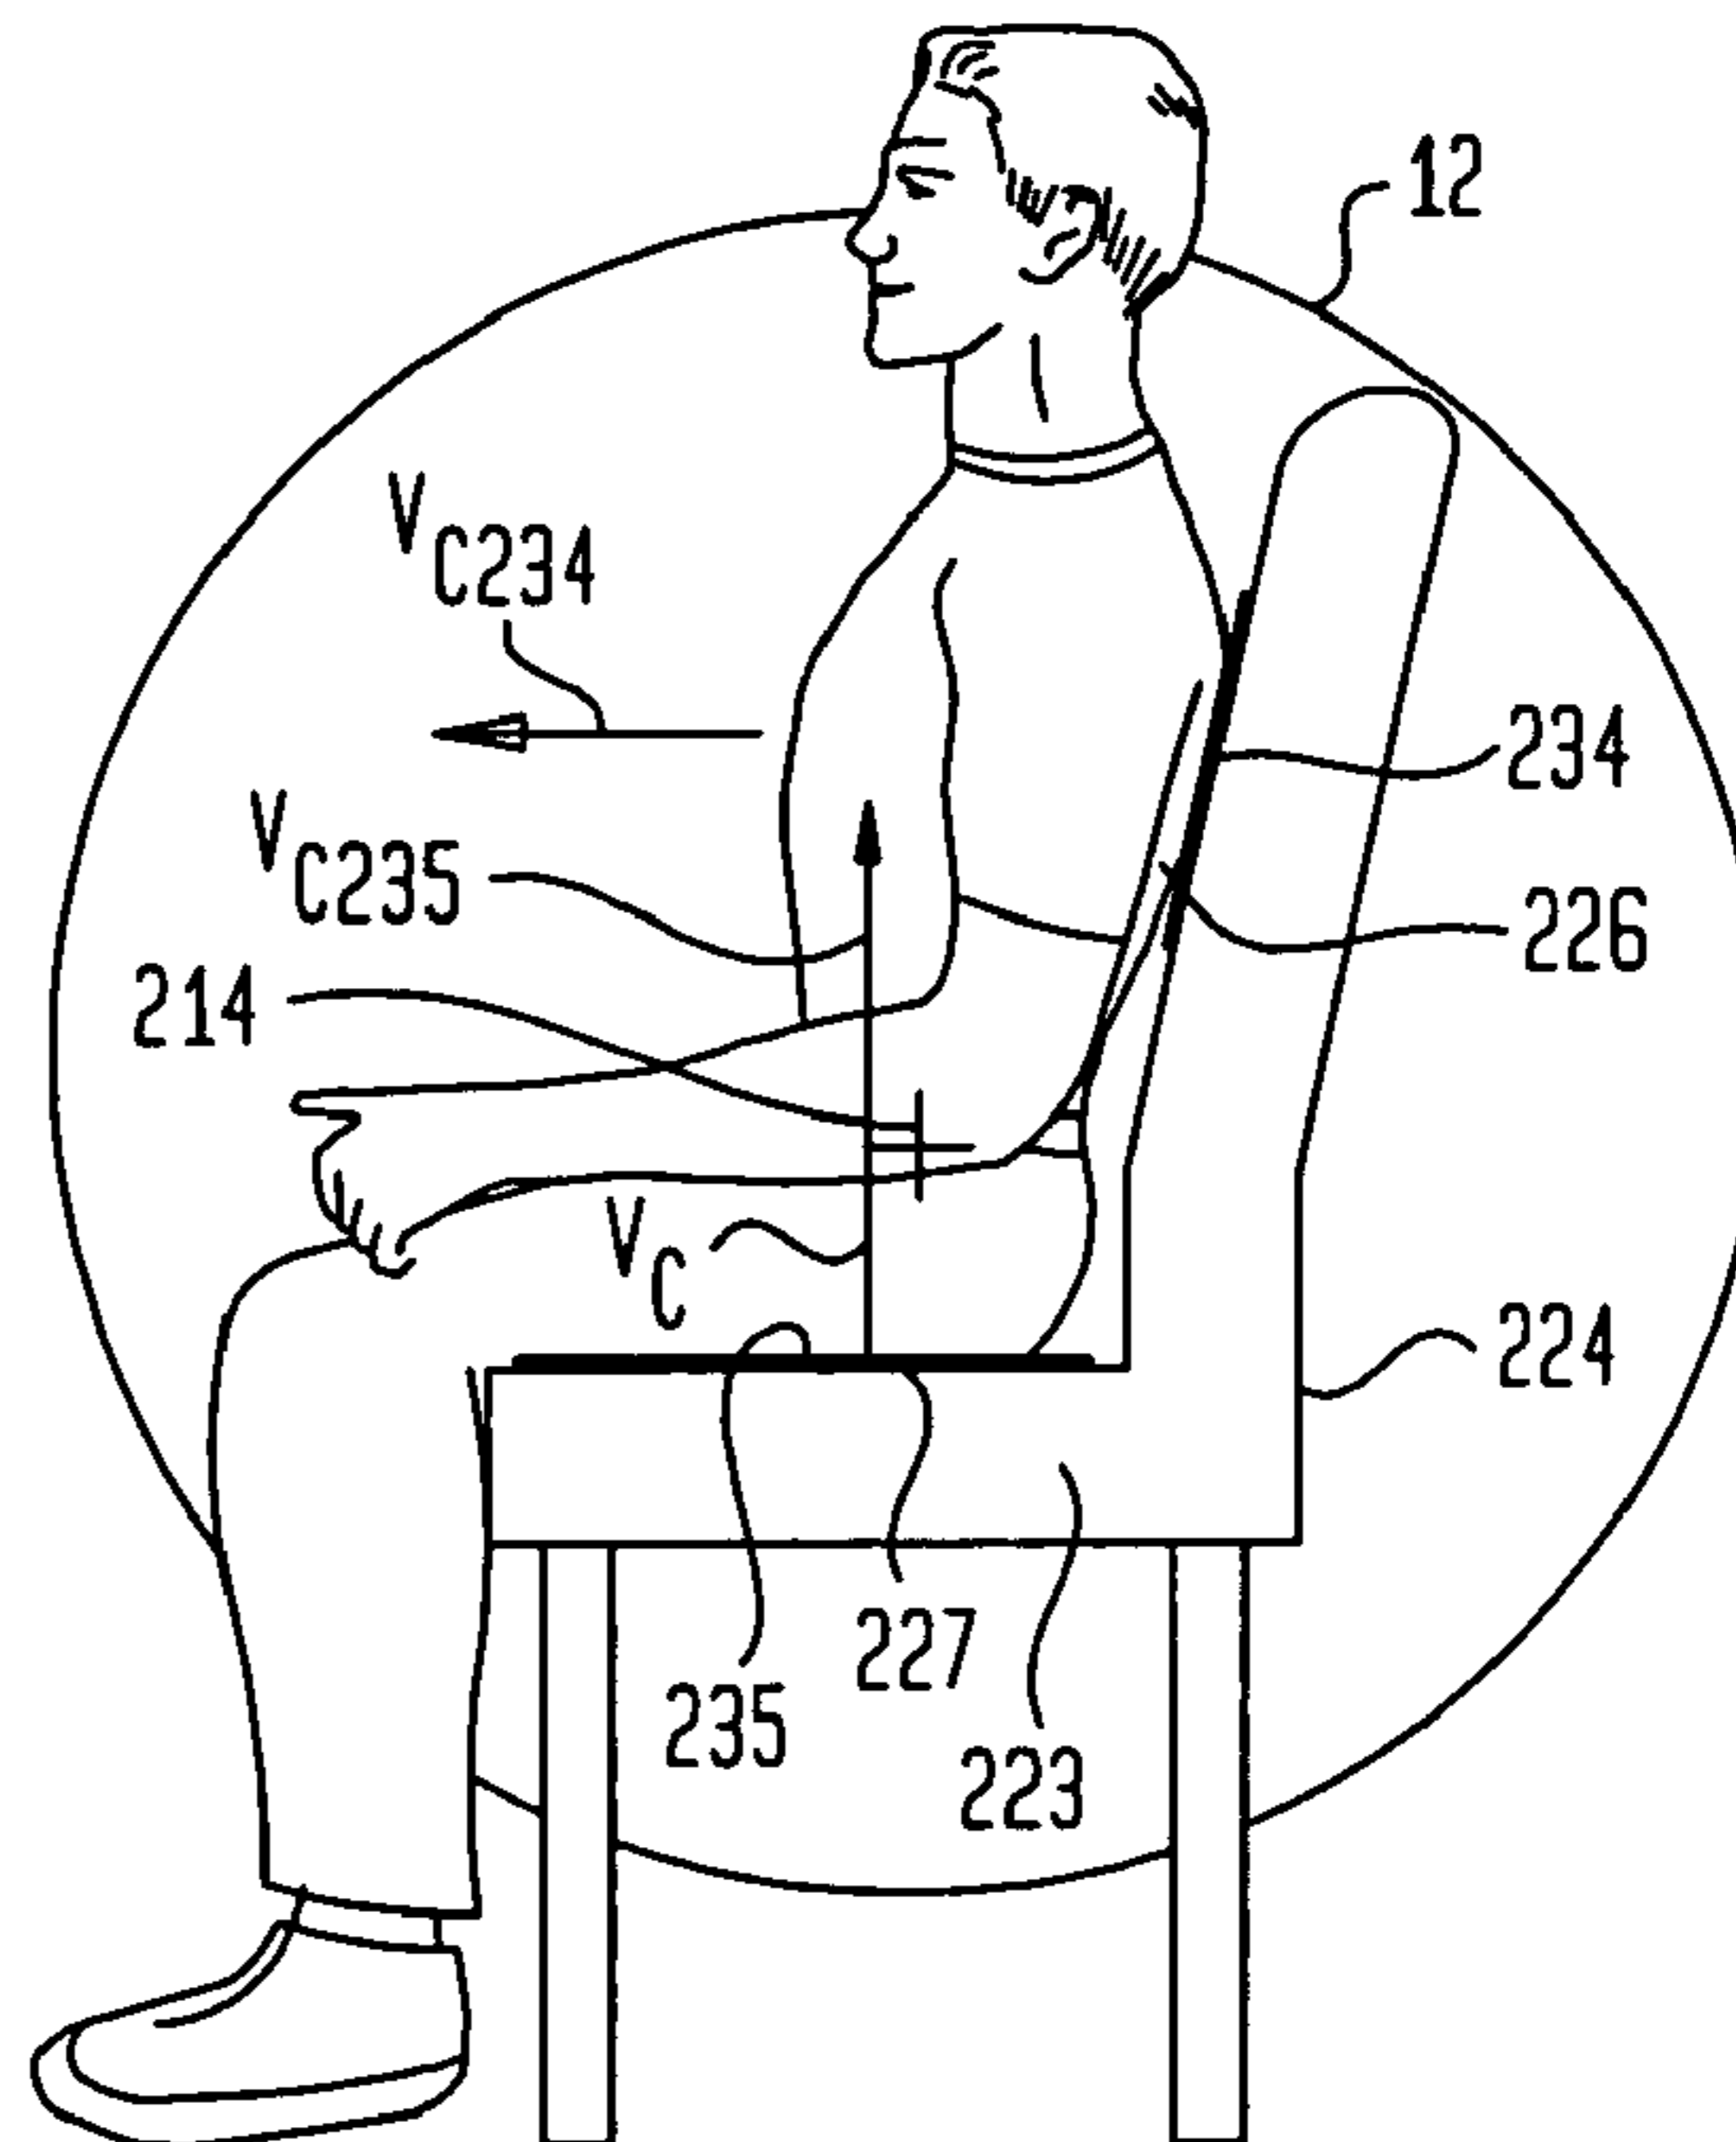


FIG. 8



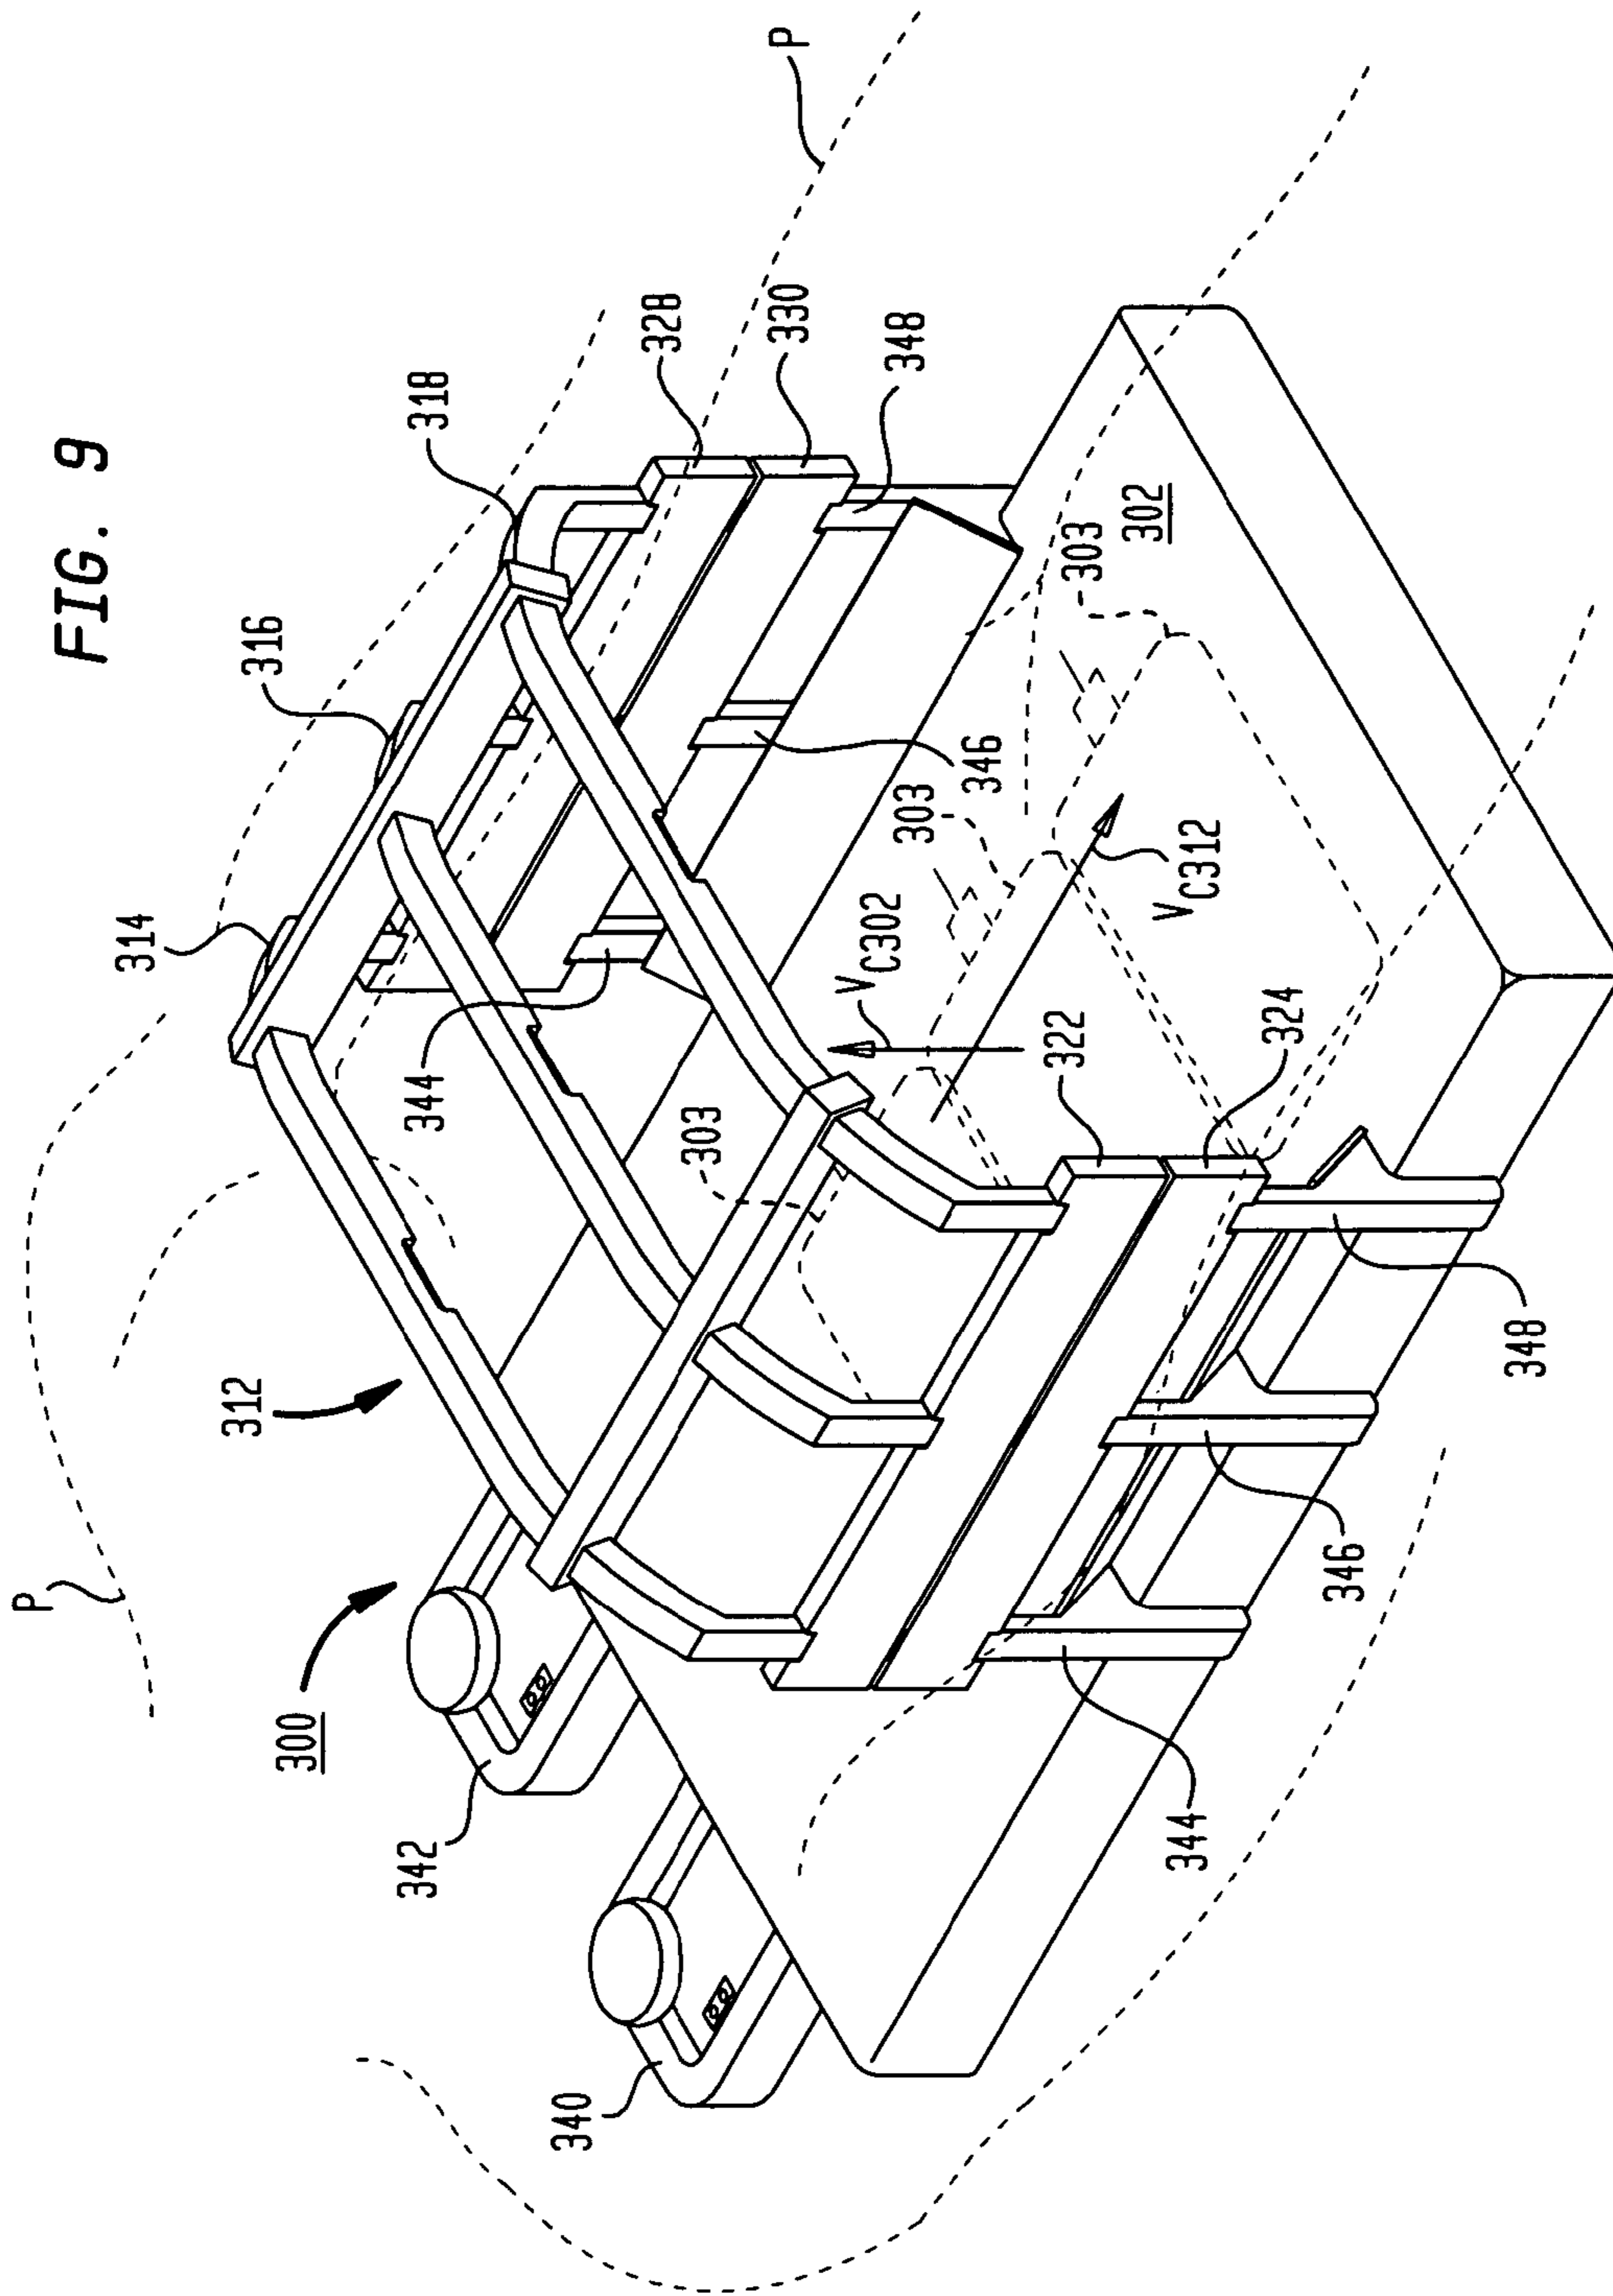


FIG. 9A

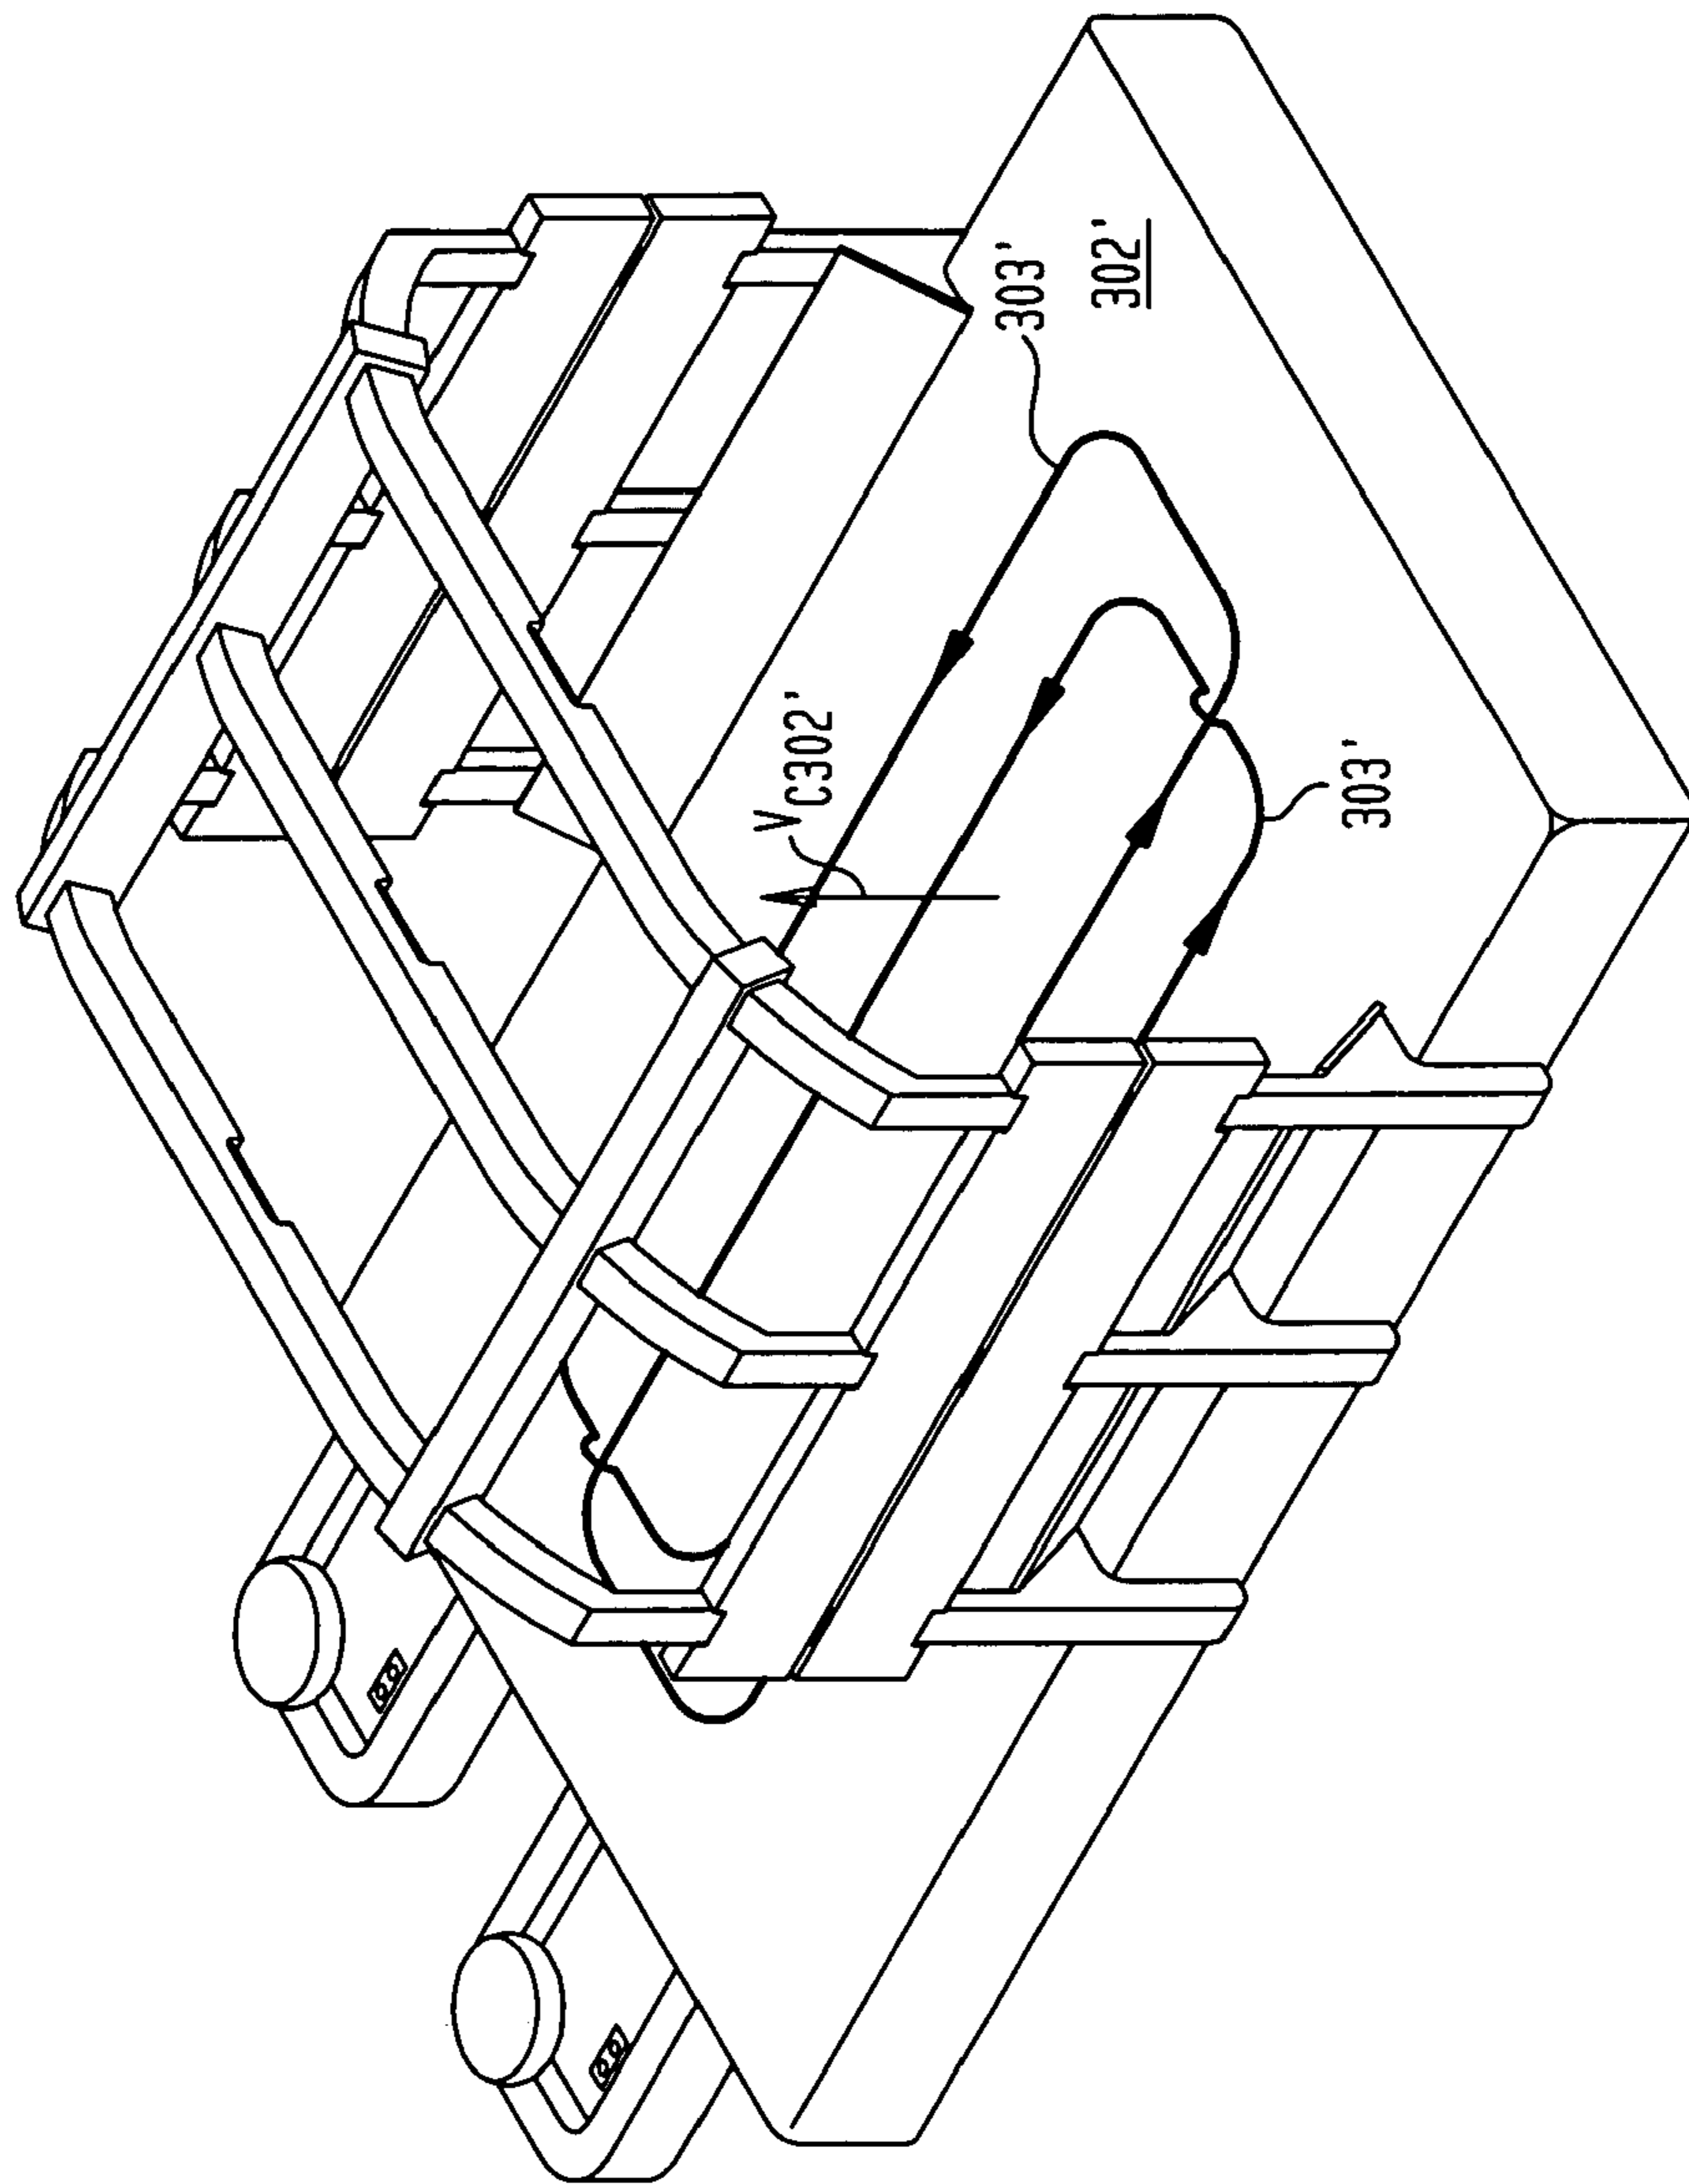


FIG. 10

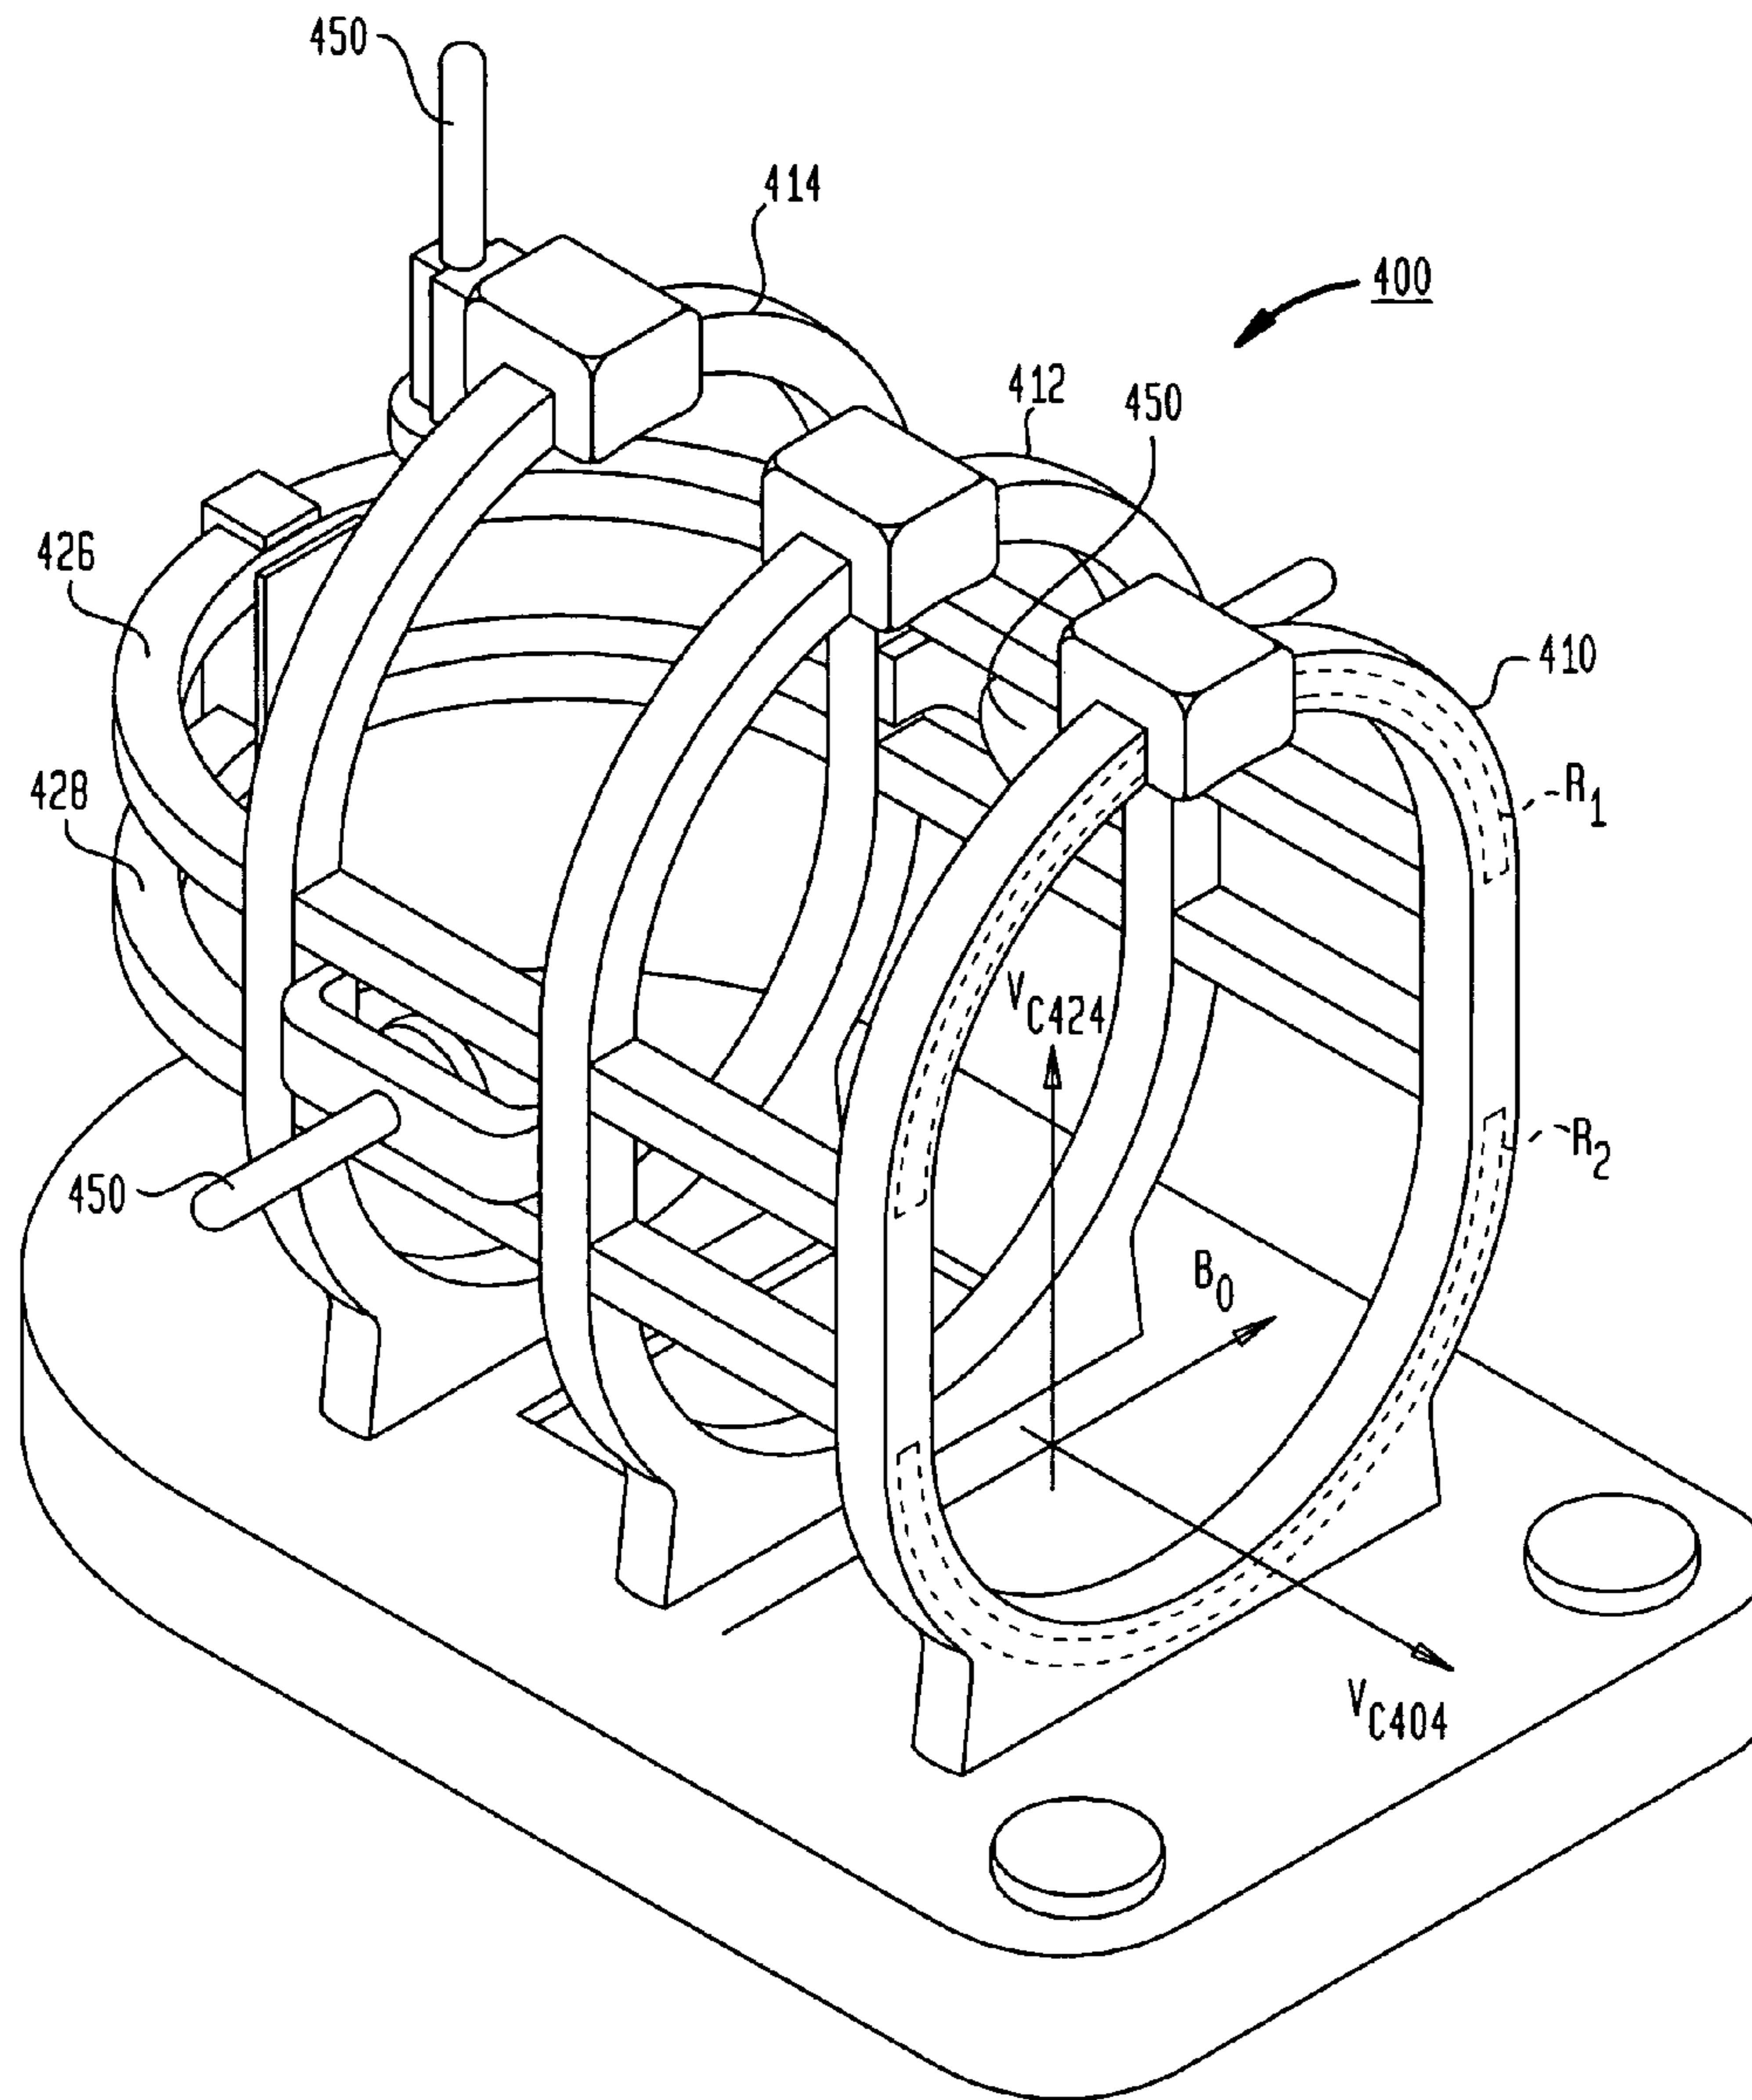


FIG. 11A

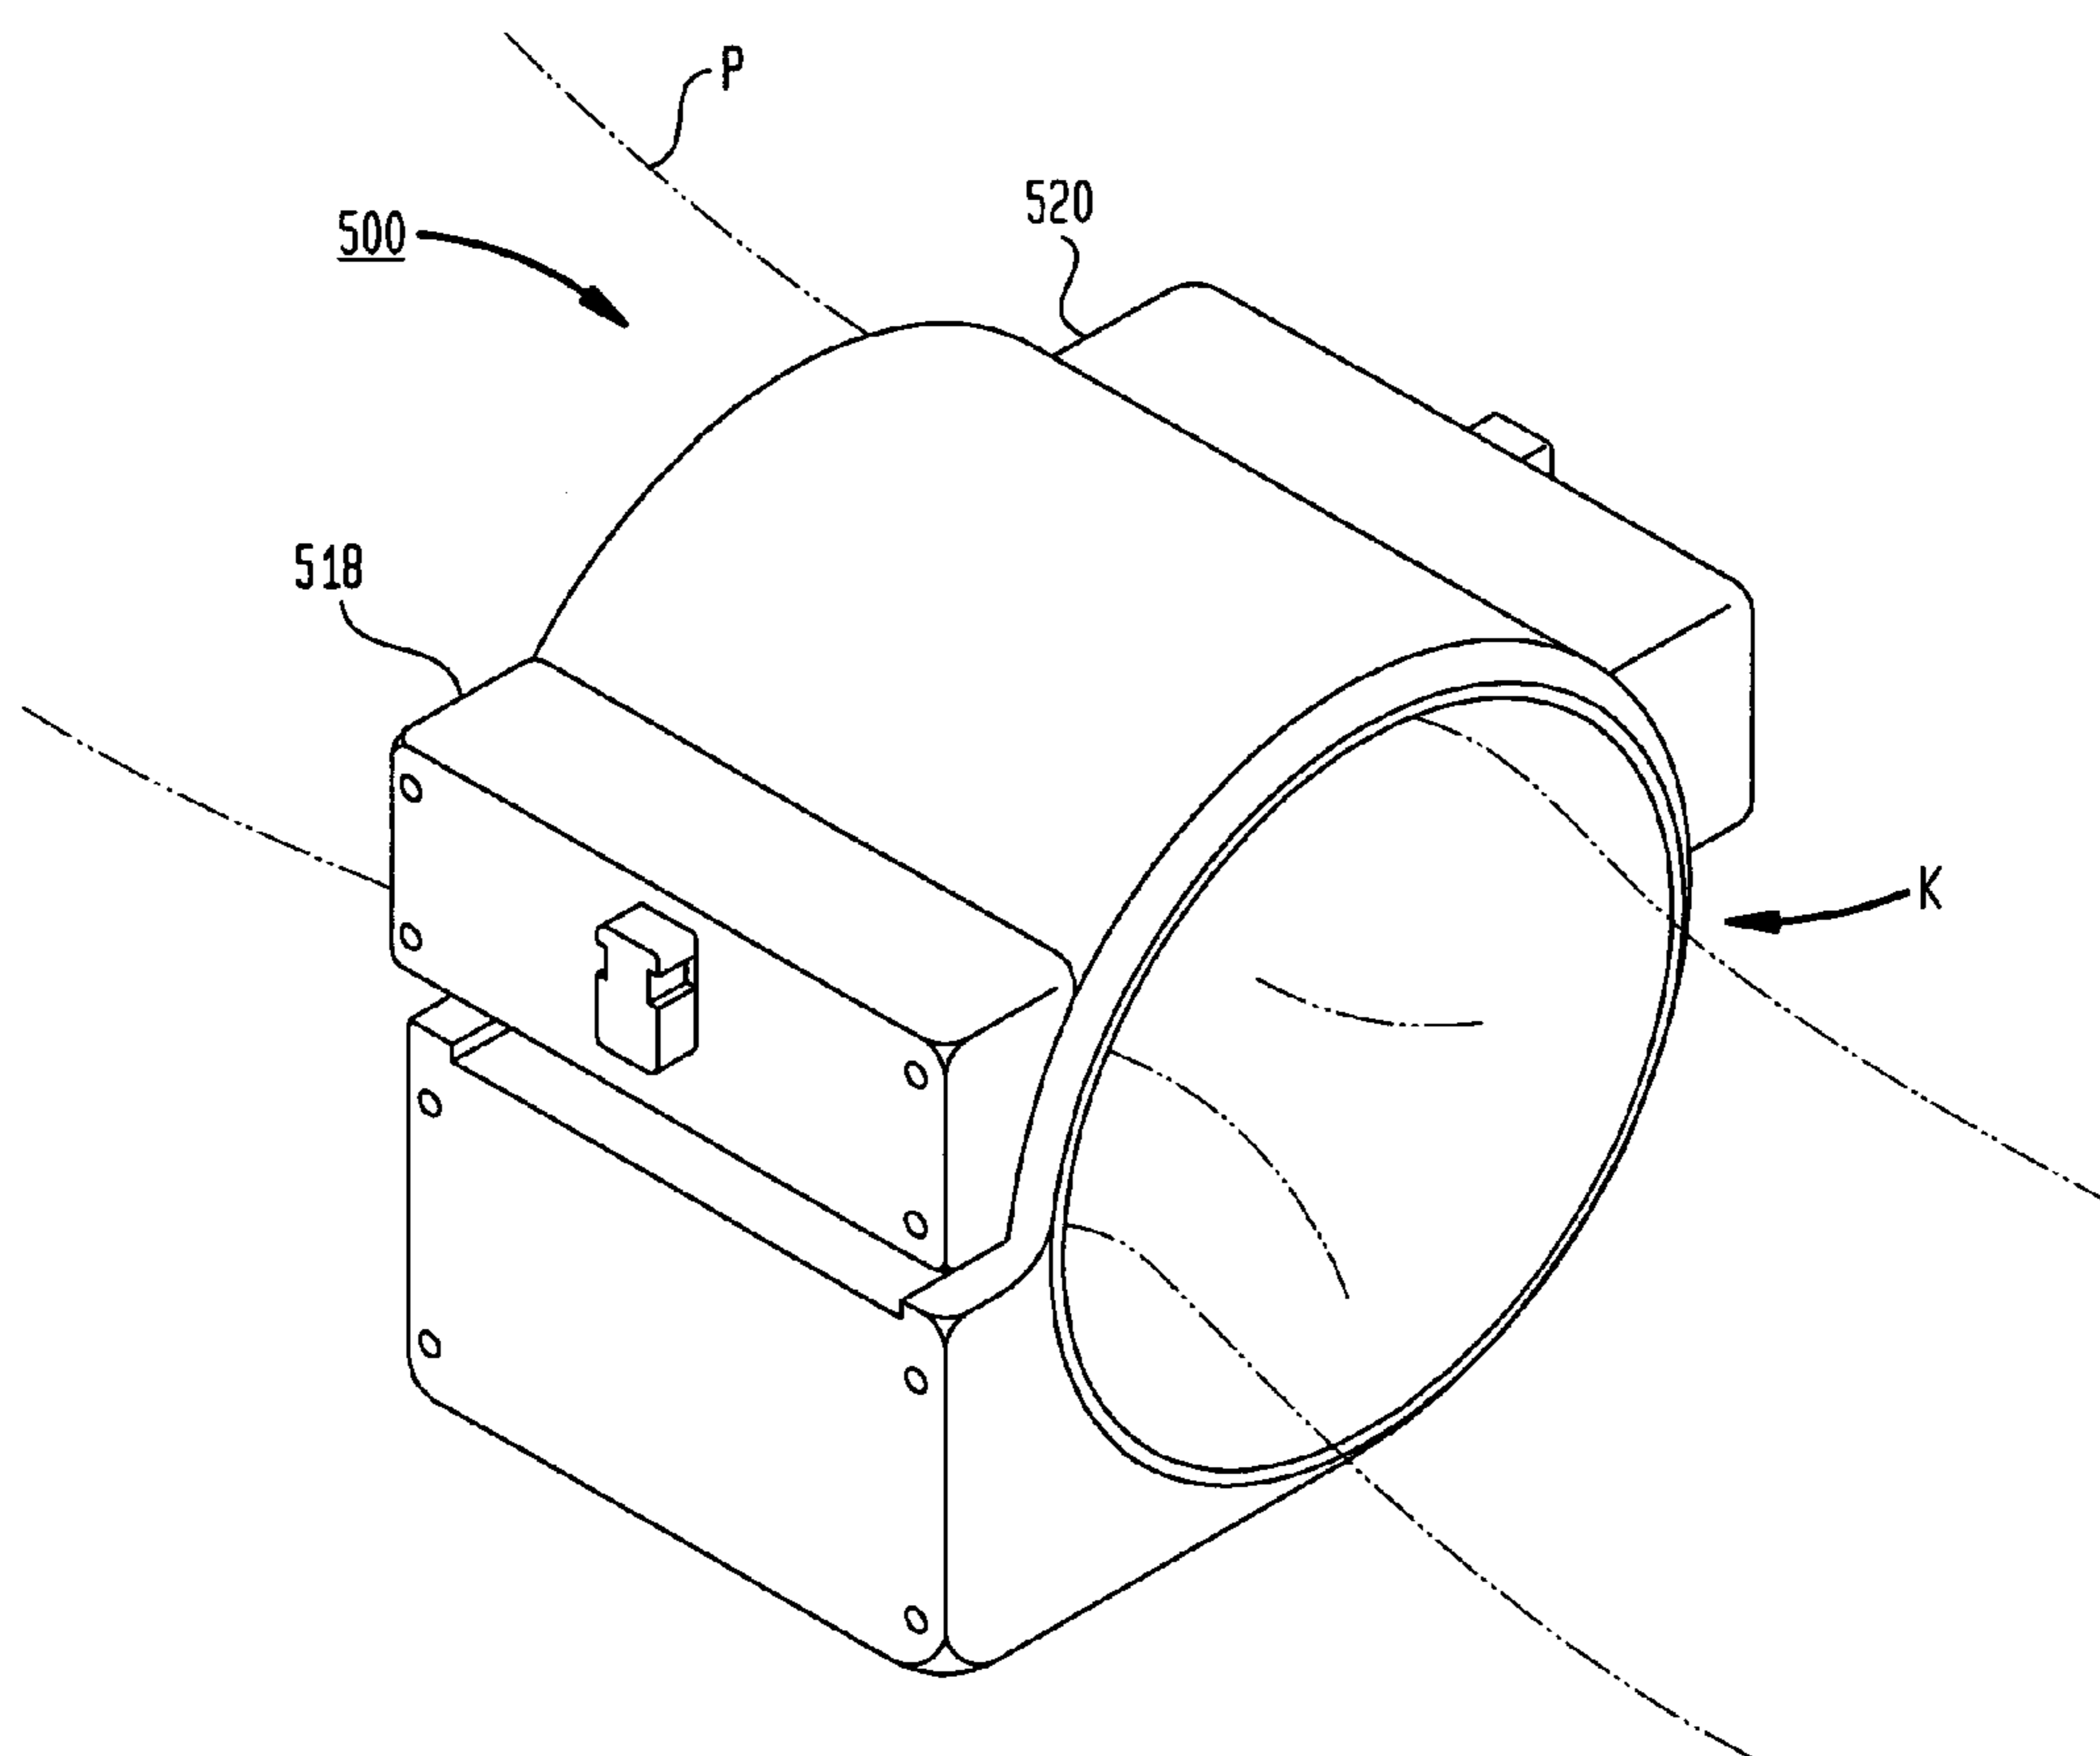


FIG. 11B

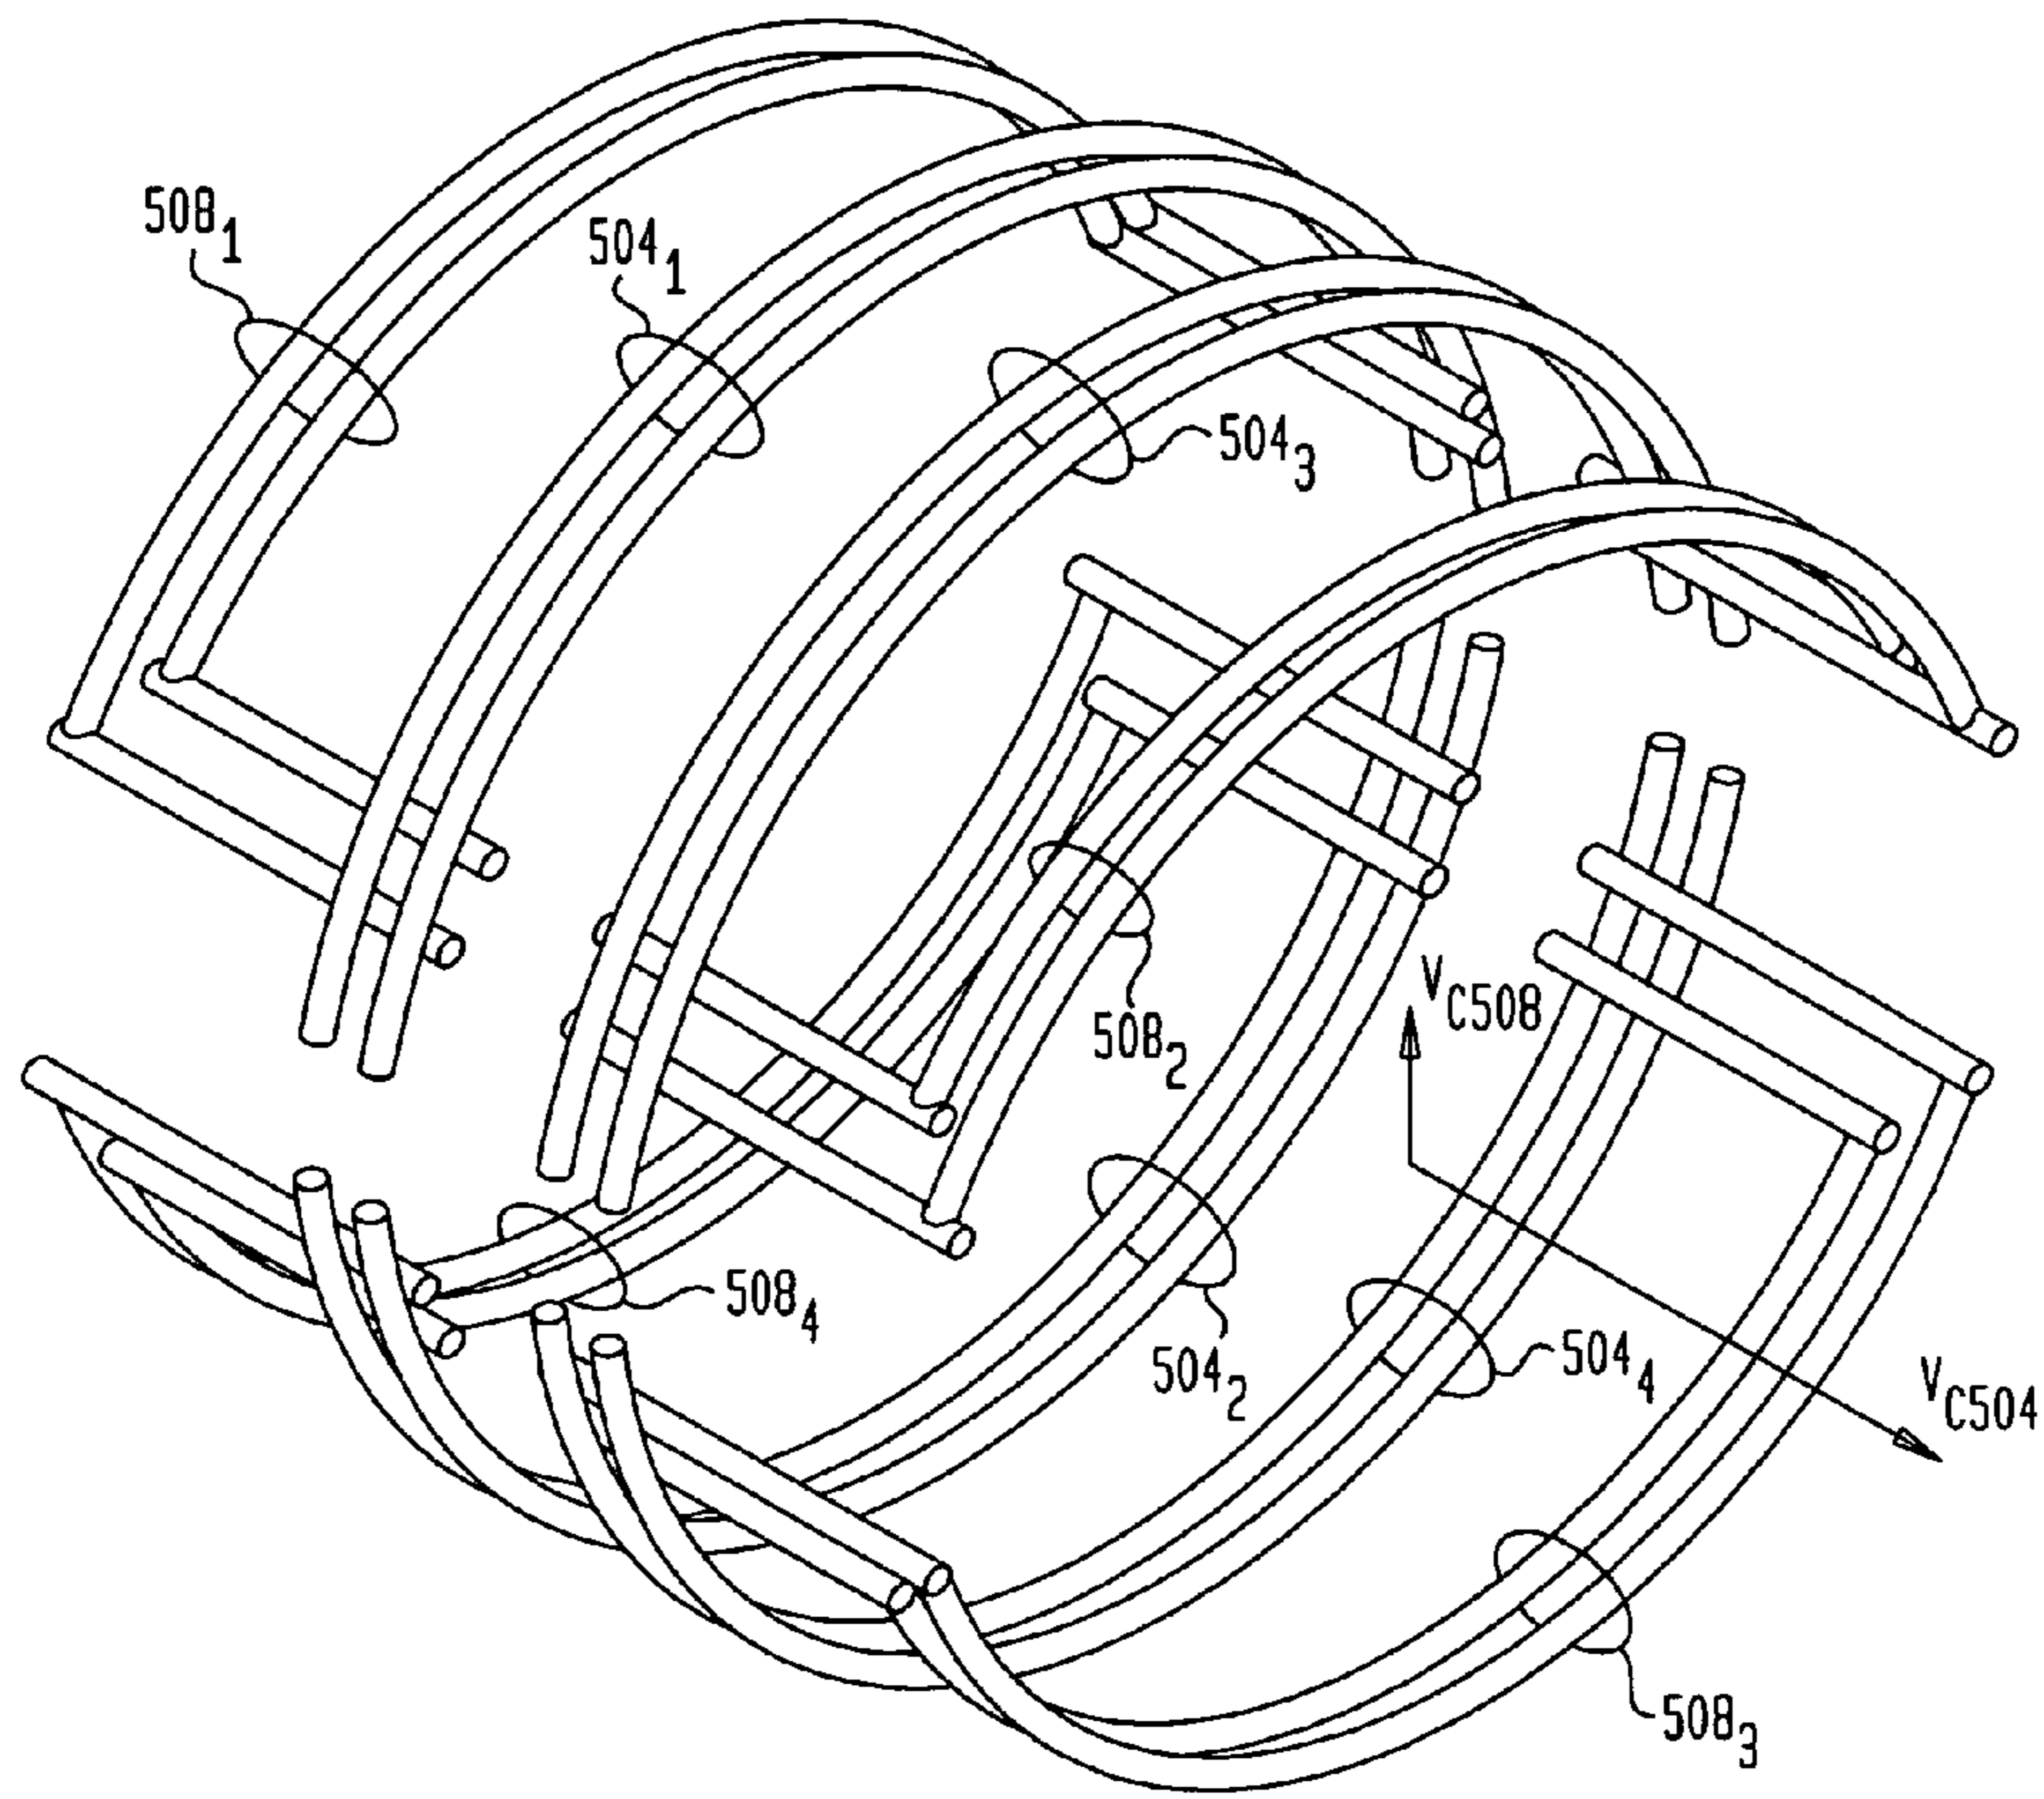
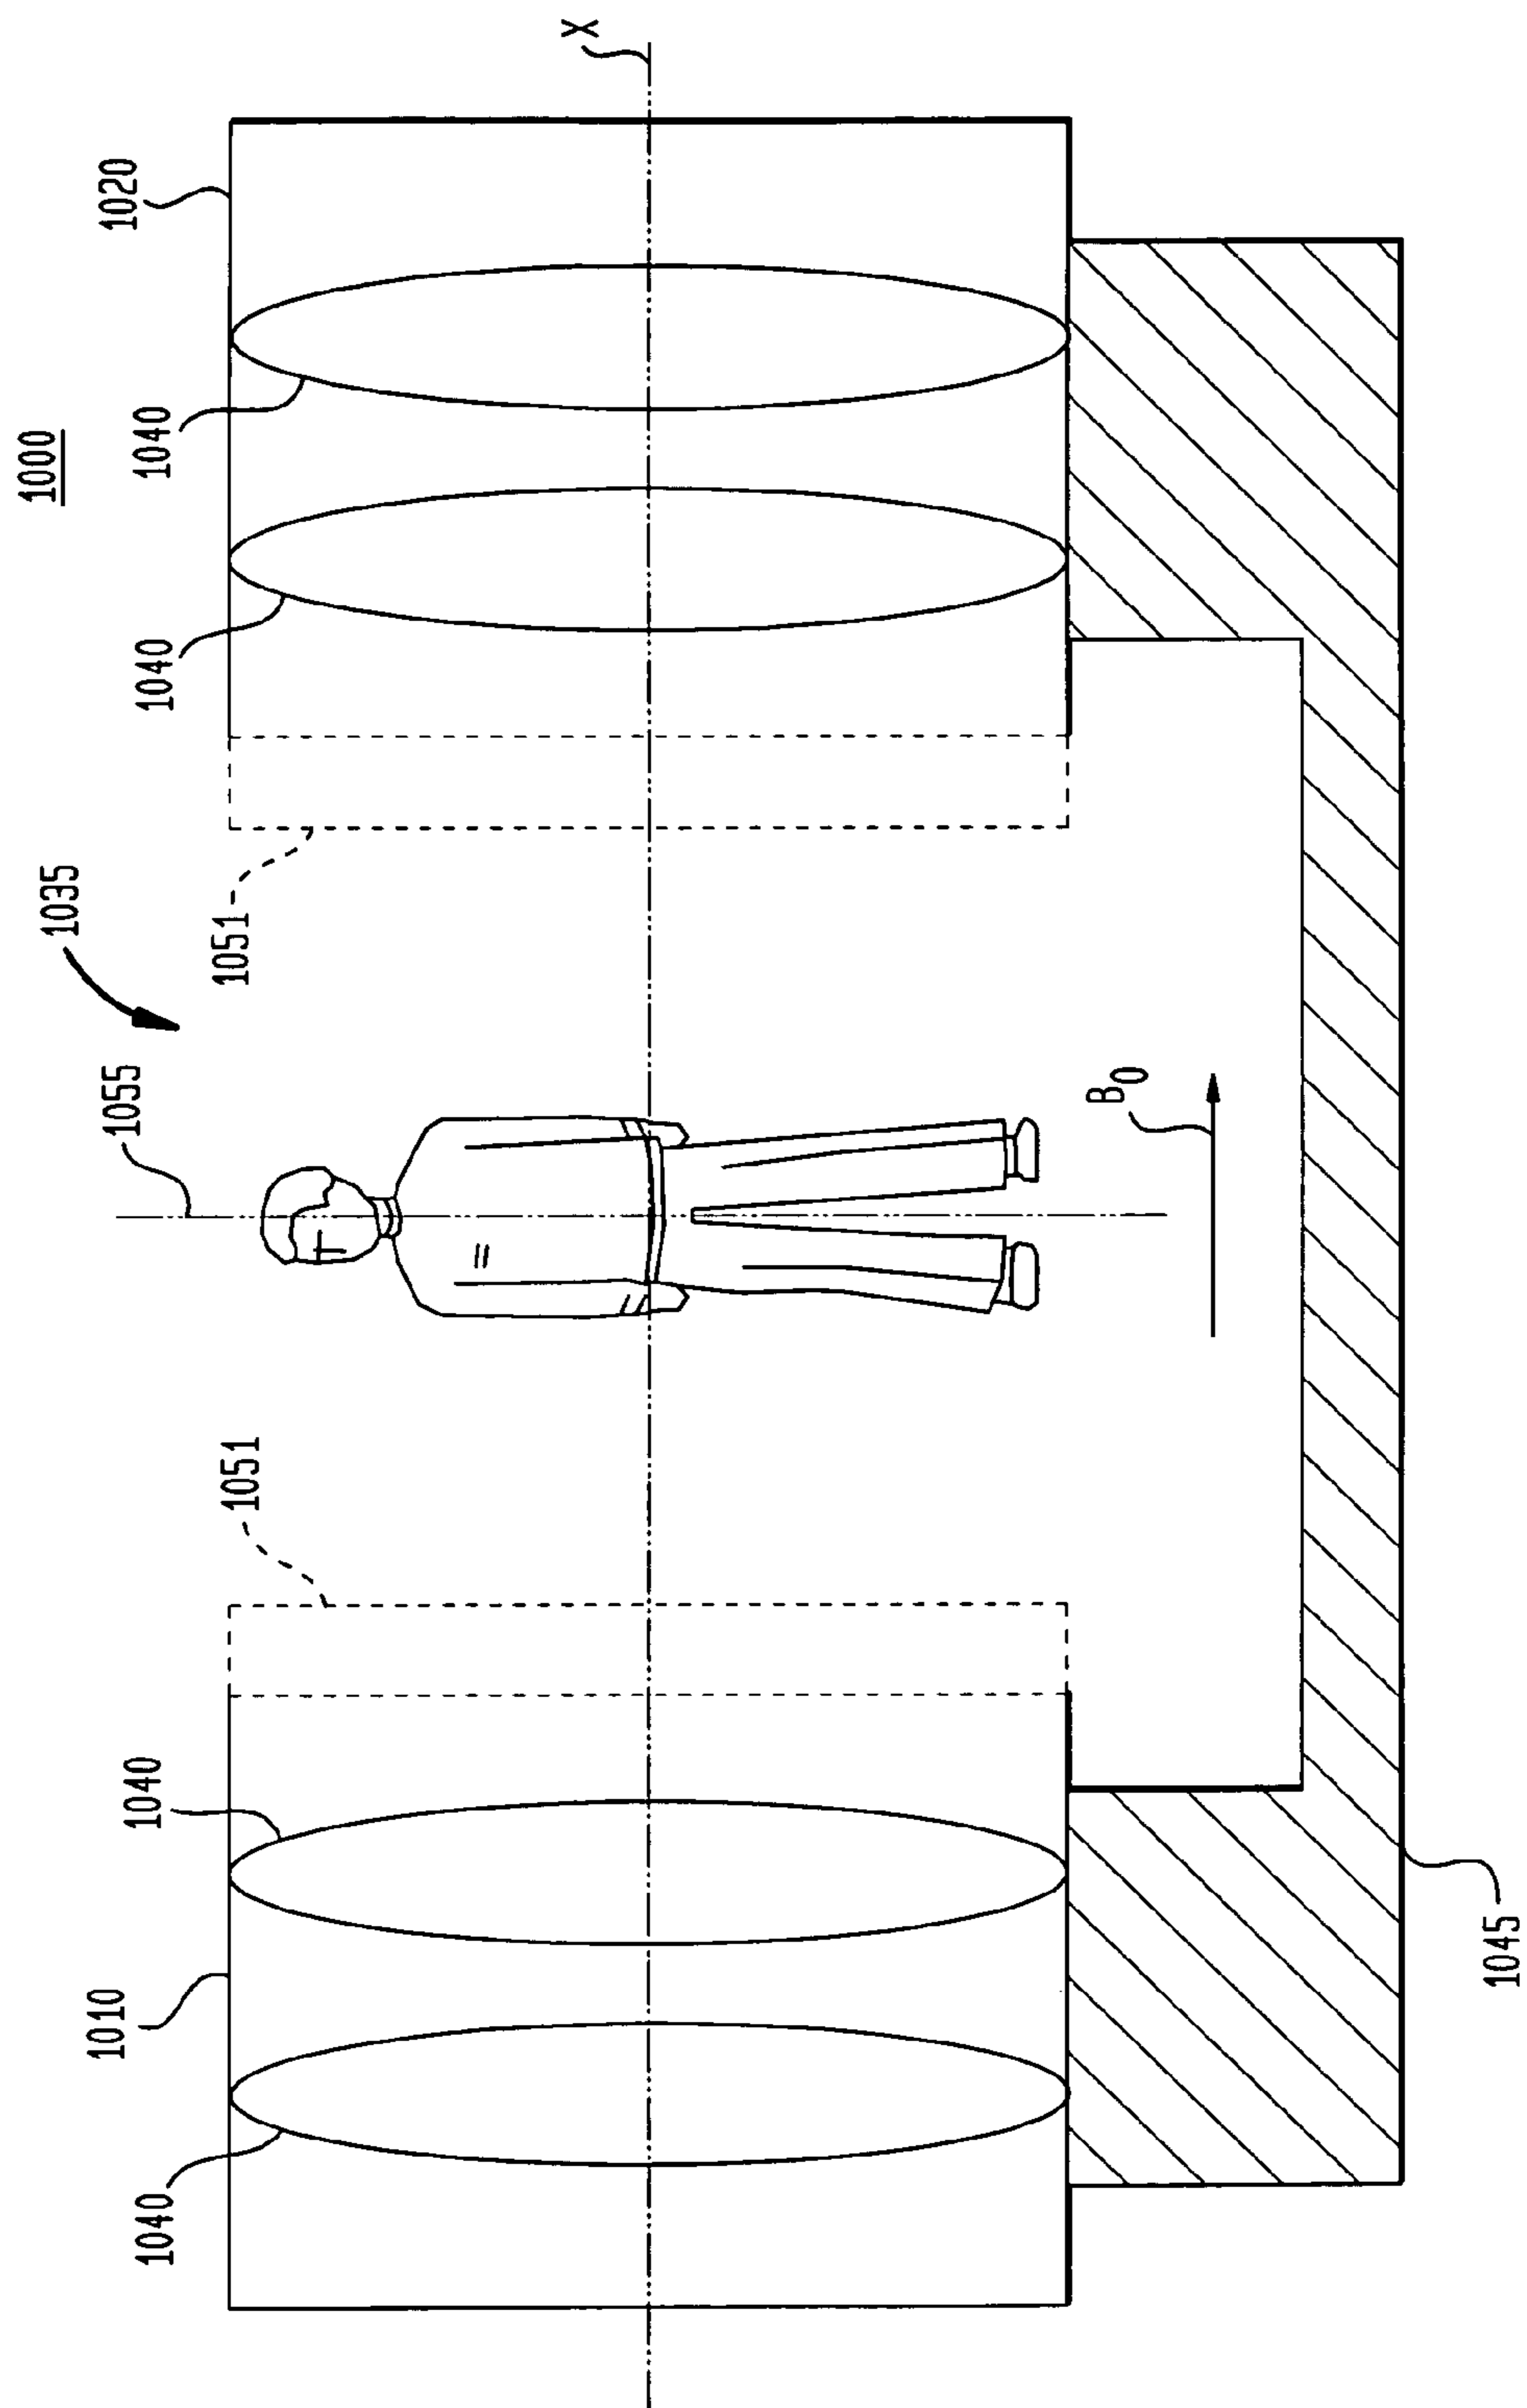


FIG. 12



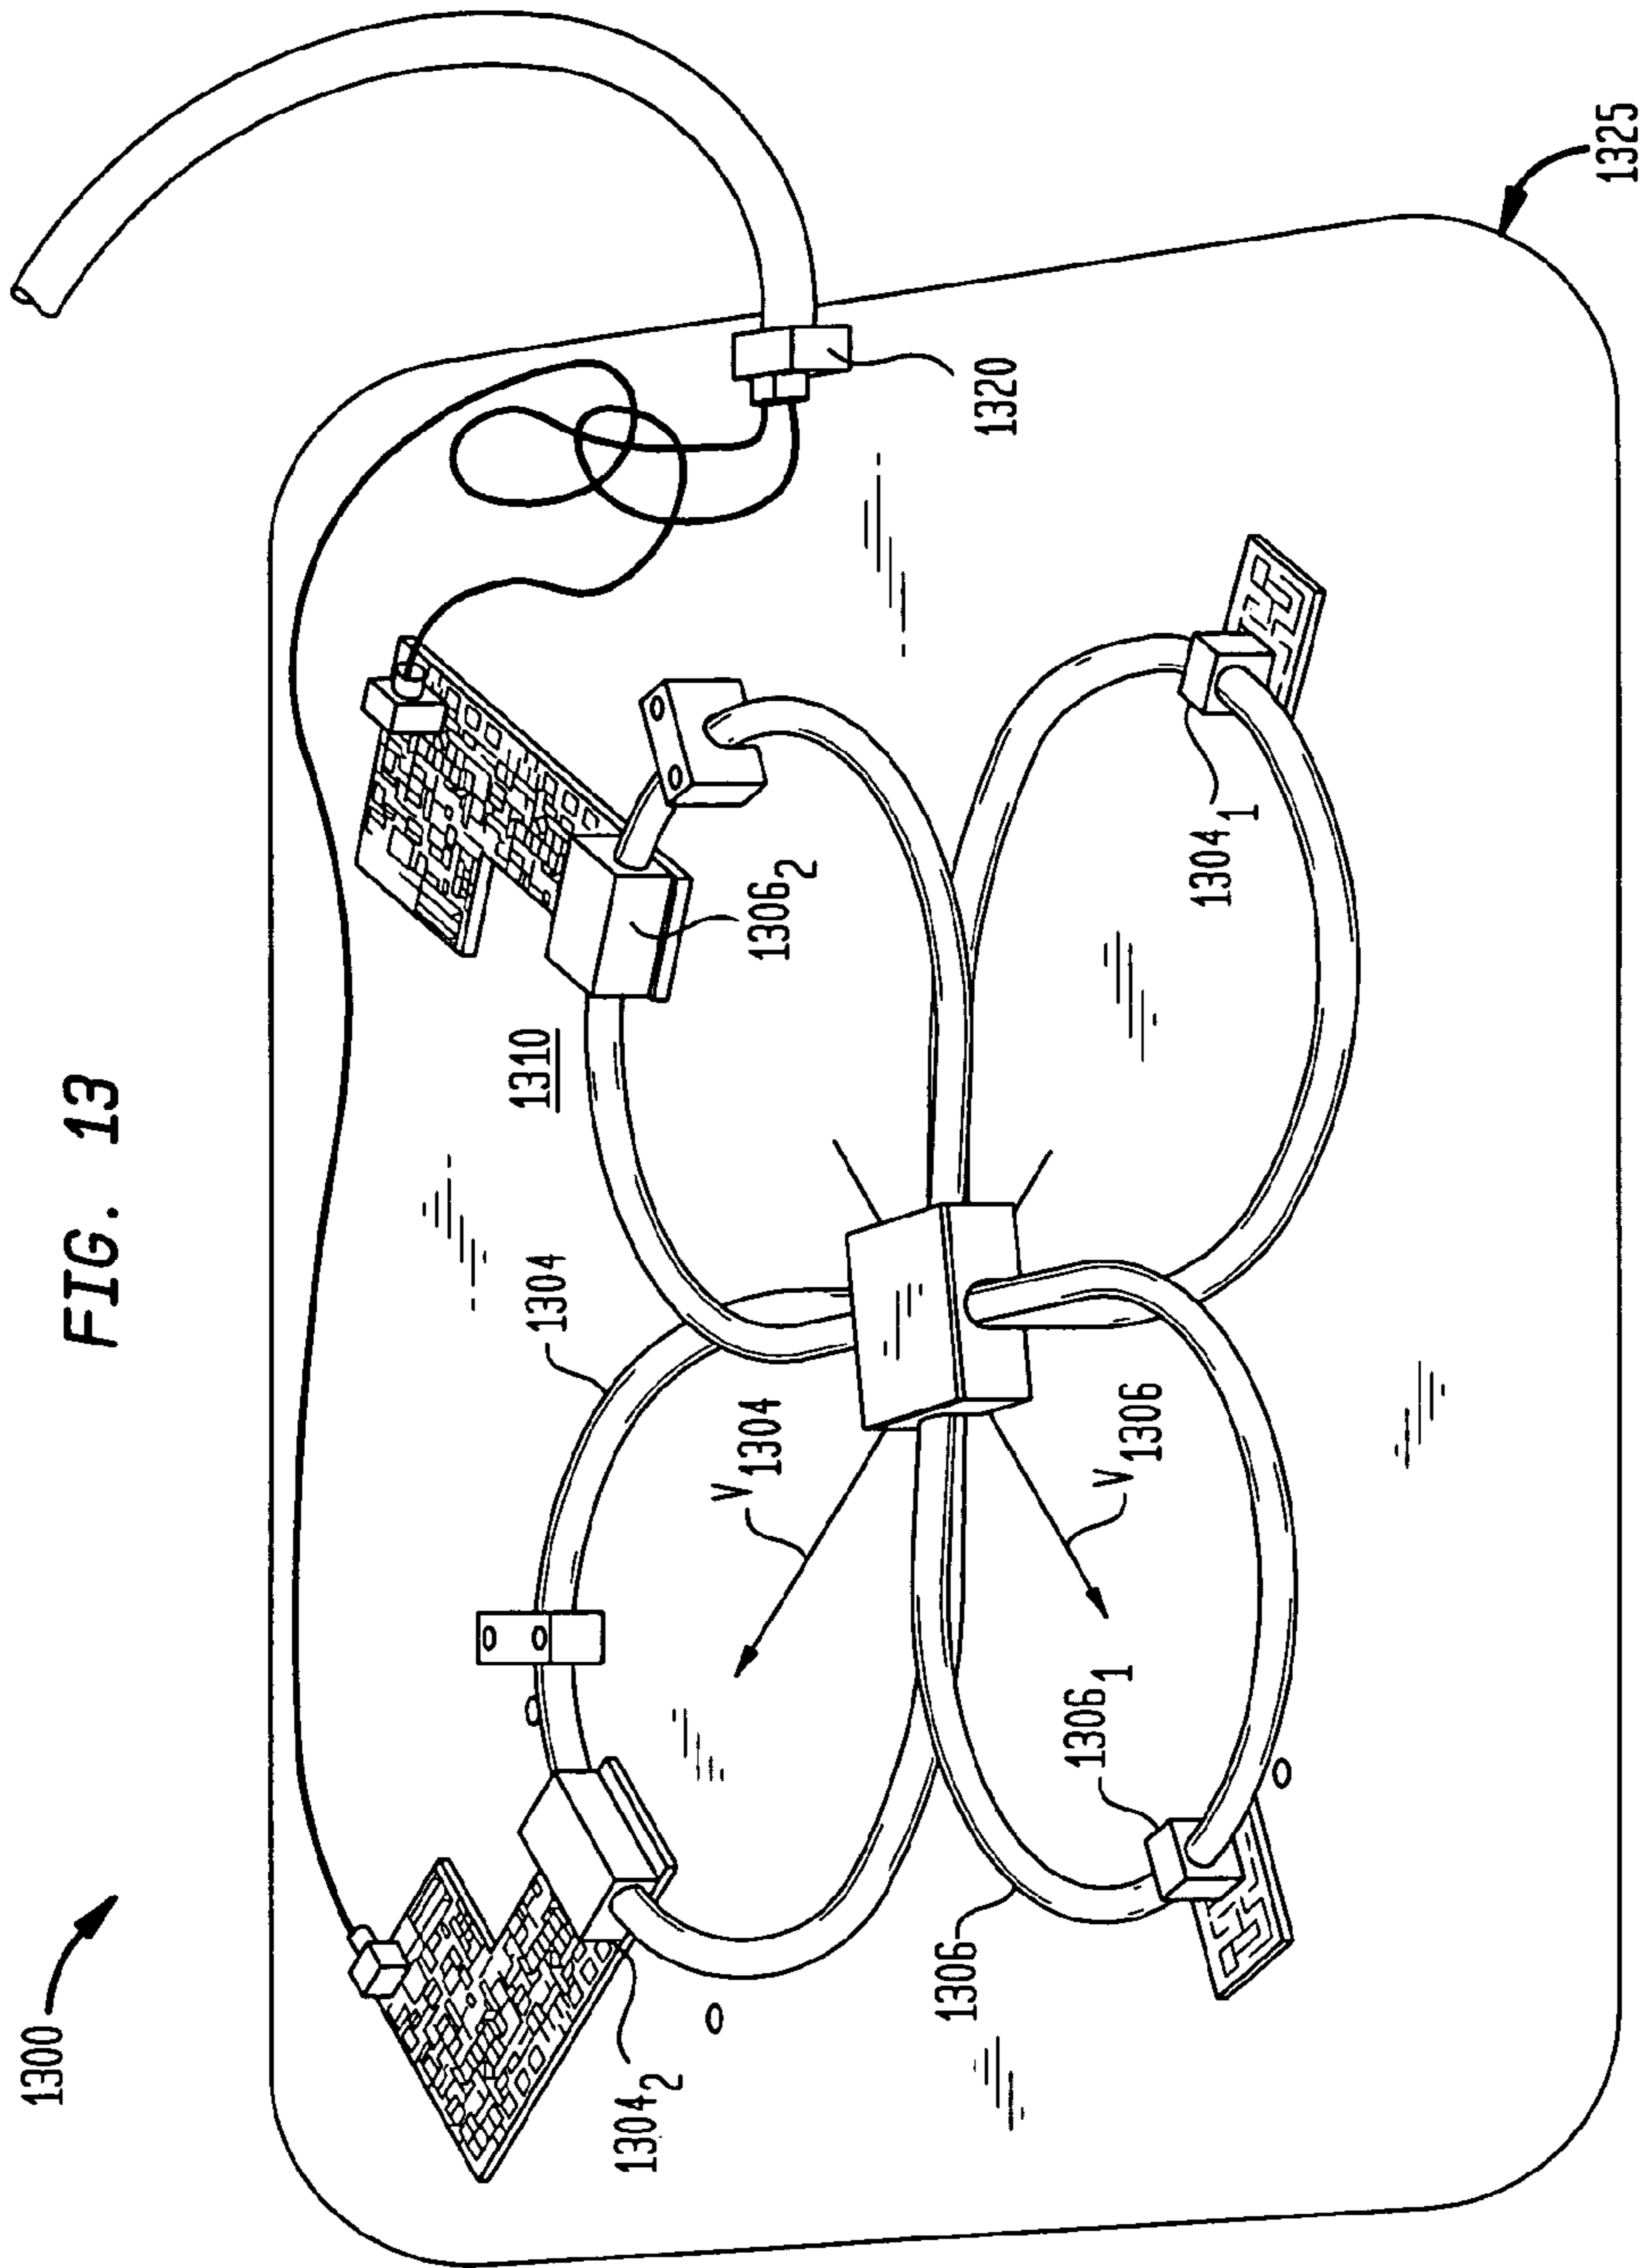


FIG. 13



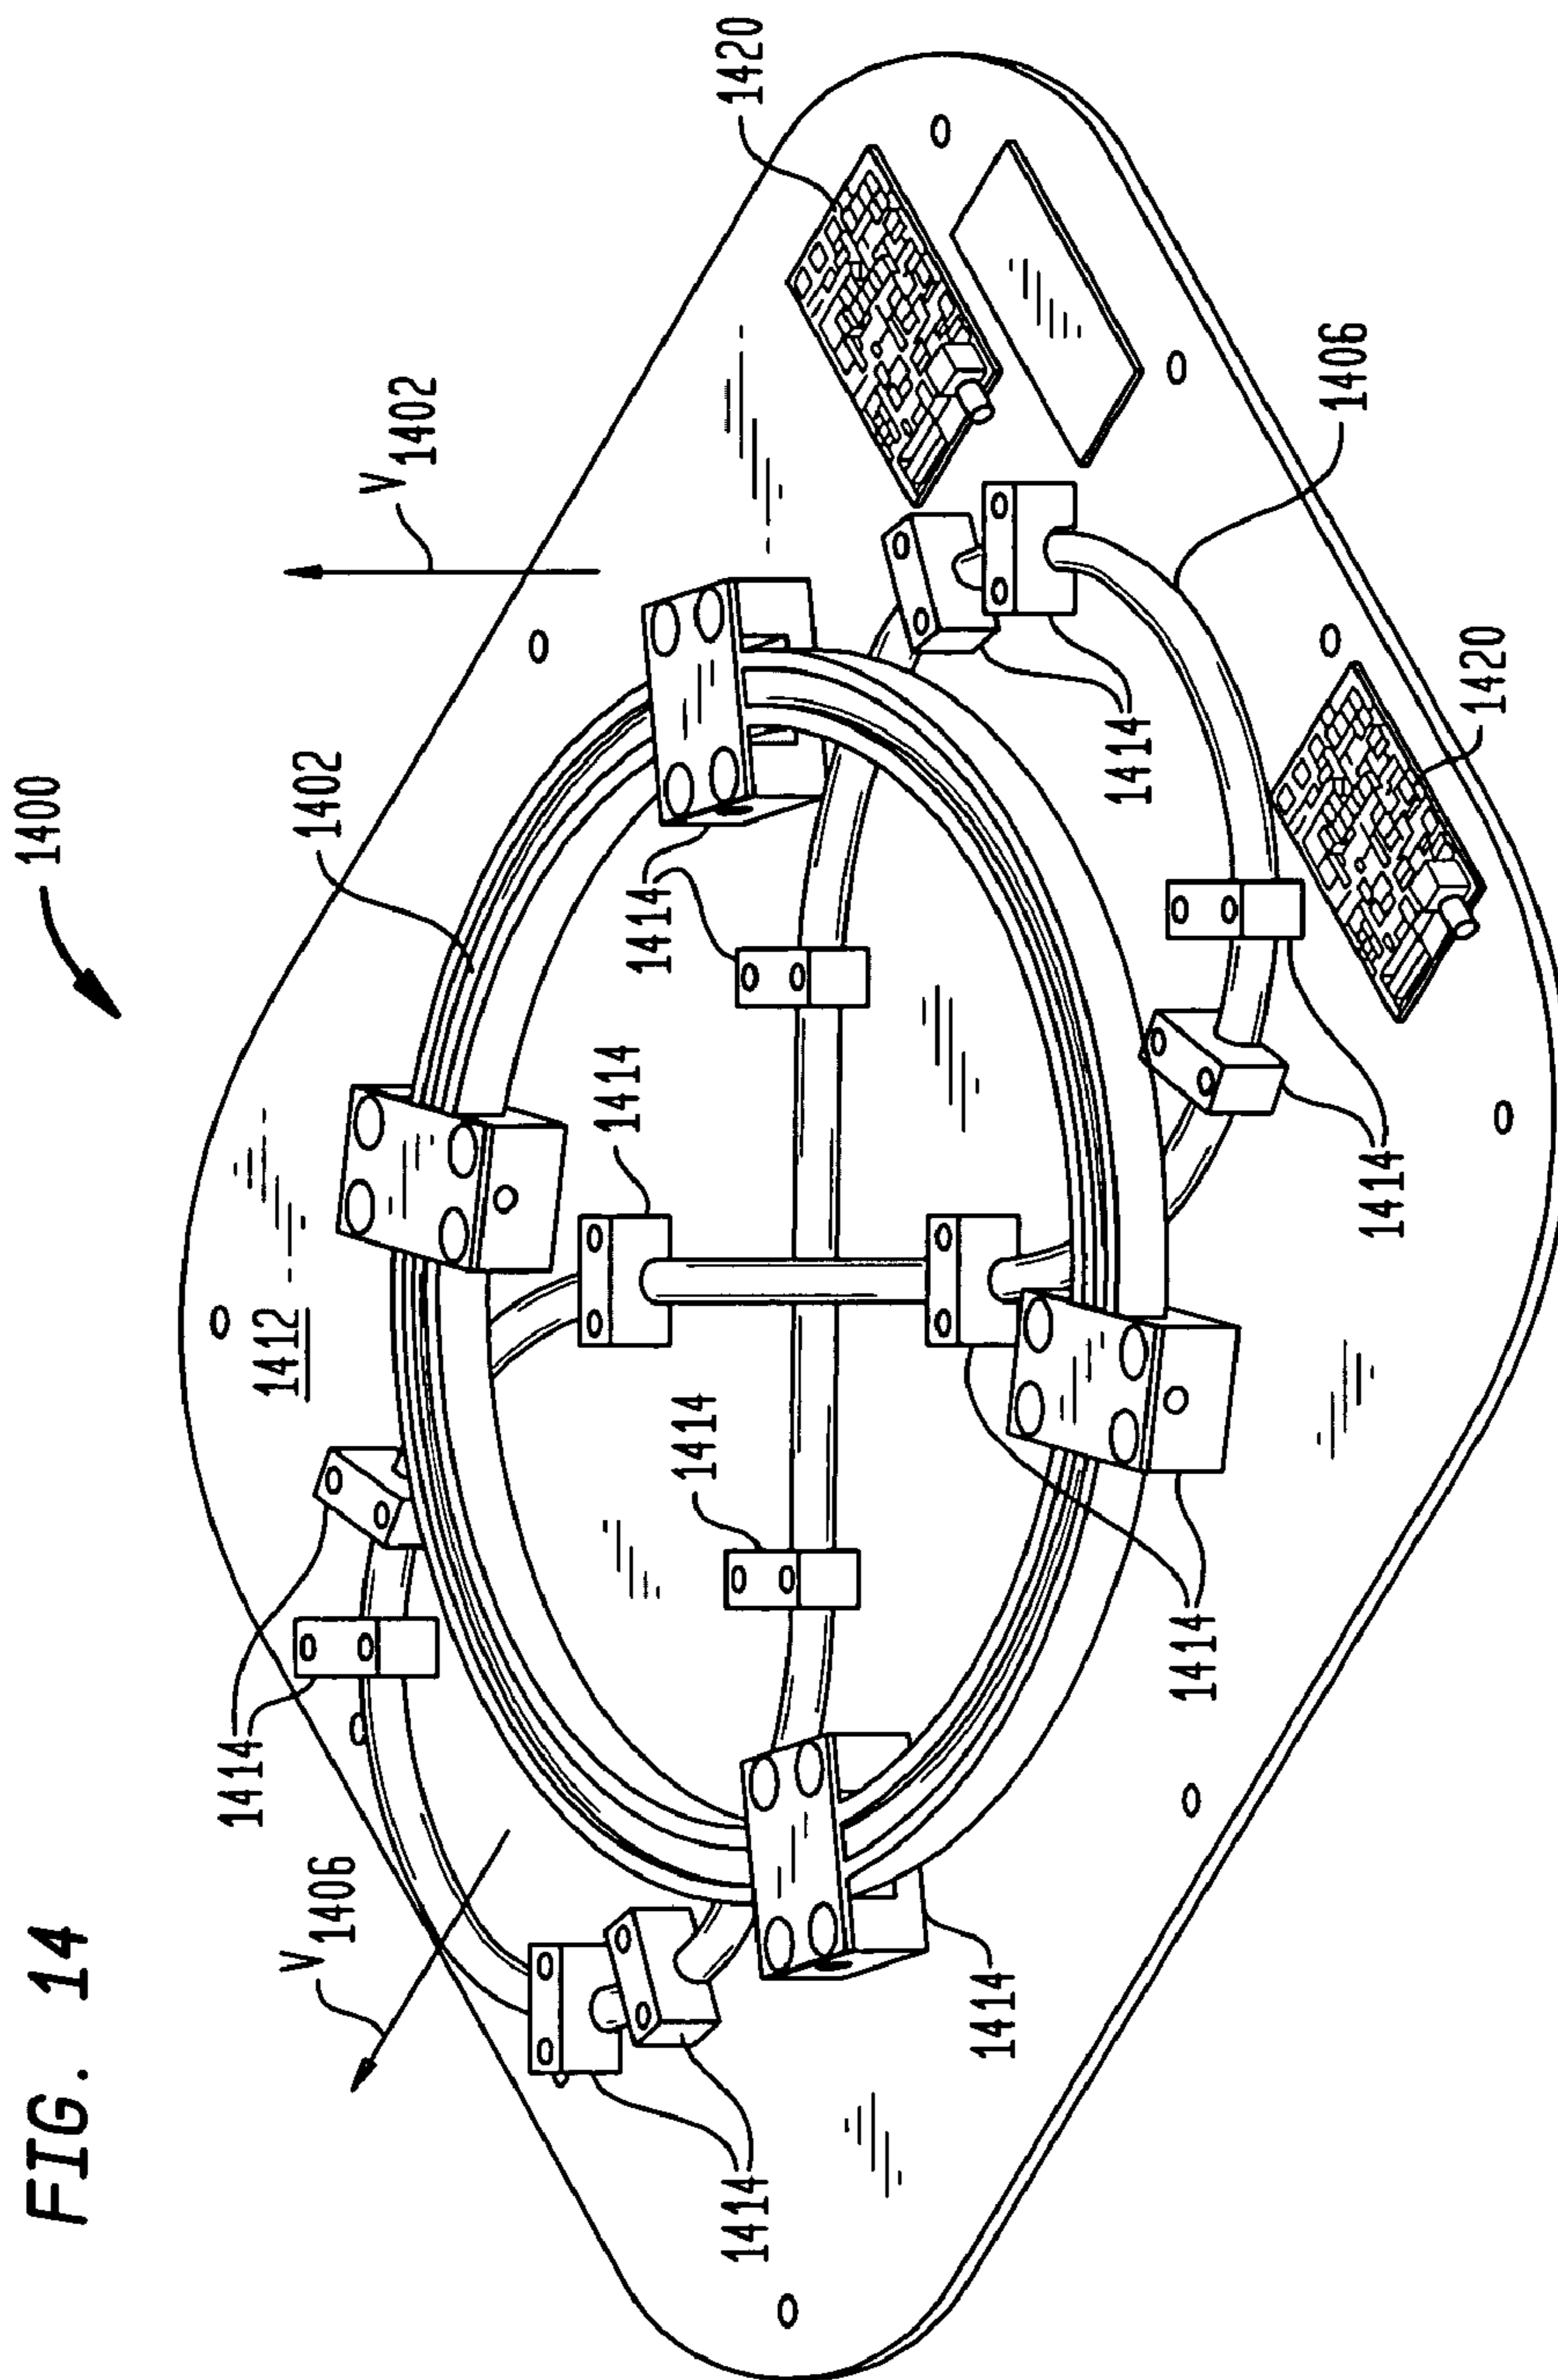


FIG. 14

## COILS FOR HORIZONTAL FIELD MAGNETIC RESONANCE IMAGING

### CROSS REFERENCE TO RELATED APPLICATIONS

The present application is a continuation-in-part of U.S. application Ser. No. 10/266,070, filed Oct. 7, 2002, entitled "Coils For Horizontal Field Magnetic Resonance Imaging" and claims the benefit of the filing date of U.S. Provisional Application Nos. 60/327,329, filed Oct. 5, 2001 and 60/342,832, filed Dec. 20, 2001, the disclosures of which are hereby incorporated herein by reference.

### BACKGROUND

The present invention relates to magnetic resonance imaging apparatus and procedures. In magnetic resonance imaging, an object to be imaged as, for example, a body of a human subject, is exposed to a strong, substantially constant static magnetic field. Radio frequency excitation energy is applied to the body, and this energy causes the spin vectors of certain atomic nuclei within the body to rotate or "precess" around axes parallel to the direction of the static magnetic field. The precessing atomic nuclei emit weak radio frequency signals during the relaxation process, referred to herein as magnetic resonance signals. Different tissues produce different signal characteristics. Furthermore, relaxation times are a major factor in determining signal strength. In addition, tissues having a high density of certain nuclei will produce stronger signals than tissues with a low density of such nuclei. Relatively small gradients in the magnetic field are superimposed on the static magnetic field at various times during the process so that magnetic resonance signals from different portions of the patient's body differ in phase and/or frequency. If the process is repeated numerous times using different combinations of gradients, the signals from the various repetitions together provide enough information to form a map of signal characteristics versus location within the body. Such a map can be reconstructed by conventional techniques well known in the magnetic resonance imaging art, and can be displayed as a pictorial image of the tissues as known in the art.

The magnetic resonance imaging technique offers numerous advantages over other imaging techniques. MRI does not expose either the patient or medical personnel to X-rays and offers important safety advantages. Also, magnetic resonance imaging can obtain images of soft tissues and other features within the body which are not readily visualized using other imaging techniques. Accordingly, magnetic resonance imaging has been widely adopted in the medical and allied arts.

Several factors impose significant physical constraints in the positioning of patients and ancillary equipment in MRI imaging. Many MRI magnets use one or more solenoidal superconducting coils to provide the static magnetic field arranged so that the patient is disposed within a small tube running through the center of the magnet. The magnet and tube typically extend along a horizontal axis, so that the long axis or head-to-toe axis of the patient's body must be in a horizontal position during the procedure. Moreover, equipment of this type provides a claustrophobic environment for the patient. Iron core magnets have been built to provide a more open environment for the patient. These magnets typically have a ferromagnetic frame with a pair of ferromagnetic poles disposed one over the other along a vertical pole axis with a gap between them for receiving the patient. The frame includes ferromagnetic flux return members such as plates or

columns extending vertically outside of the patient-receiving gap. A magnetic field is provided by permanent magnets or electromagnetic coils associated with the frame. A magnet of this type can be designed to provide a more open environment for the patient. However, it is still generally required for the patient to lie with his or her long axis horizontal.

Recently, ferromagnetic frame magnets having horizontal pole axes have been developed. As disclosed, for example, in commonly assigned U.S. patent application Ser. No. 08/978,084, filed on Nov. 25, 1997, and U.S. Pat. Nos. 6,414,490 and 6,677,753, the disclosures of which are incorporated by reference herein, a magnet having poles spaced apart from one another along a horizontal axis provides a horizontally oriented magnetic field within a patient-receiving gap between the poles. Such a magnet can be used with a patient positioning device including elevation and tilt mechanisms to provide extraordinary versatility in patient positioning. For example, where the patient positioning device includes a bed or similar device for supporting the patient in a recumbent position, the bed can be tilted and/or elevated so as to image the patient in essentially any position between a fully standing position and a fully recumbent position, and can be elevated so that essentially any portion of the patient's anatomy is disposed within the gap in an optimum position for imaging. As further disclosed in the aforesaid applications, the patient positioning device may include additional elements such as a platform projecting from the bed to support the patient when the bed is tilted towards a standing orientation. Still other patient supporting devices can be used in place of a bed in a system of this type. For example, a seat may be used to support a patient in a sitting position. Thus, magnets of this type provide extraordinary versatility in imaging.

Another physical constraint on MRI imaging has been posed by the requirements for RF antennas to transmit the RF excitation energy and to receive the magnetic resonance signals from the patient. The antenna that receives the signals is positioned near that portion of the patient's body that is to be imaged so as to maximize the signal-to-noise ratio and improve reception of the weak magnetic resonance signals. The antenna that applies RF excitation energy can be positioned in a similar location to maximize efficiency of the applied RF energy. In some cases, the same antenna is used to apply RF excitation energy and to receive the magnetic resonance signals at different times during the process. However, it is often desirable to provide two separate antennas for this purpose.

The antennas are typically formed as one or more loops of electrically conductive material. Such a loop antenna must be positioned so that the conductor constituting the loop extends along an imaginary plane or surface having a normal vector transverse to the direction of the static magnetic field. Stated another way, the antenna must be arranged to transmit or receive electromagnetic fields in a direction perpendicular to the direction of the static magnetic field if it is to interact with the precessing atomic nuclei. This requirement has further limited available antenna configurations and techniques. For example, in a vertical-field magnet such as a ferromagnetic frame magnet having a vertical pole axis, it is impossible to use a loop antenna with the loop disposed generally in a horizontal plane below the body of a recumbent patient. Such an antenna has a normal vector which is vertical and hence parallel to the direction of the static magnetic field. A loop antenna which encircles the patient with its normal vector extending horizontally can be employed. Also, planar or saddle-shaped loops extending in generally vertical planes or surfaces, and having normal vectors in the horizontal direction transverse to the long axis of the patient can be positioned

3

on opposite sides of the patient. However, these antenna configurations do not provide optimum signal-to-noise ratios in some procedures as, for example, in imaging the spine, head or pelvic region.

#### SUMMARY OF THE INVENTION

In accordance with an embodiment of the present invention an apparatus for magnetic resonance imaging comprises a magnet having a patient-receiving space and a horizontal pole axis. The magnet desirably includes a source of magnetic flux that provides a static magnetic field with a field vector in a substantially horizontal direction. A patient-positioning and antenna assembly is used in combination with the magnet to position and image the region of the patient's anatomy which is of interest within the patient-receiving space. The patient-positioning and antenna assembly desirably includes a patient support having a support surface adapted to support a surface of a human body. The antenna assembly preferably includes a first antenna including one or more coils, at least some of the coils extending along coil surfaces substantially parallel to the support surface and adjacent thereto, whereby a surface of a body supported by the support surface will closely overlie the coils. The patient-positioning and antenna assembly further includes a frame for holding the patient support so that a vector normal to the support surface and the coil surface extends transverse to the pole axis and transverse to said field vector. In accordance with this embodiment of the present invention, the coils are positioned in close proximity to the region of the patient's anatomy to be imaged so that the image obtained provides more detailed information for analysis.

In accordance with another aspect of the present invention an apparatus for magnetic resonance imaging preferably comprises a magnet defining a patient-receiving space and having a static magnetic field with a field vector in a substantially horizontal direction. The apparatus desirably includes a quadrature coil antenna arrangement for receiving a signal from an object or patient disposed within the patient receiving space. The quadrature coil antenna includes a first antenna having a first coil vector and a second antenna having a second coil vector, the first and second coil vector being transverse to the static magnetic field vector. Further in accordance with this aspect of the present invention, the static magnetic field vector is oriented substantially transverse to the long axis of the patient disposed in the receiving space. This embodiment advantageously provides for better signal-to-noise performance during scanning through the use of the quadrature coil arrangement.

In yet another aspect in accordance with the present invention, an antenna arrangement for horizontal field magnetic resonance imaging preferably comprises a first antenna having a first coil vector and a second antenna having a second coil vector. The first and second antennas being desirably arranged so that the first coil vector and second coil vector are substantially transverse to each other. In addition, the first and second antennas are further desirably arranged so that the first coil vector and the second coil vector are substantially transverse to the horizontal magnetic field. In accordance with this aspect of the present invention, the static magnetic field vector is oriented substantially transverse to the long axis of the patient disposed in the receiving space. Images taken in accordance with this aspect of the present invention benefit from the improvement in signal-to-noise ratio which results in images having more detail for the operator, medical professional or user.

In another embodiment in accordance with the present invention, a magnetic resonance imaging apparatus prefer-

4

ably comprises a stationary magnet having a pair of elements spaced apart from one another along a horizontal axis and a patient-receiving space between the elements in combination with a quadrature coil antenna arrangement. The magnet is operable to direct magnetic flux between the elements through the patient receiving space. The antenna assembly preferably includes a first antenna having a first coil vector and a second antenna having a second coil vector. The first coil vector and second coil vector are oriented substantially transverse to the horizontal magnetic field and the horizontal magnetic field is oriented substantially transverse to the long axis of the patient disposed within the patient receiving space.

In accordance with a method aspect of the invention method for magnetic resonance imaging is provided. The method preferably comprises the steps of providing a static magnetic field in a space, the static magnetic field having a substantially horizontal magnetic field vector and positioning a patient on a patient support surface so that the patient's body preferably overlies the support and overlies one or more coils of a first antenna, the one or more coils having coil surfaces substantially parallel to the support surface and adjacent thereto. The patient support surface is then desirably positioned in the static field so that the vectors normal to the coil surfaces are substantially transverse to the field vector and magnetic resonance signals are elicited by transmitting RF energy to the body and receiving said magnetic resonance signals, at least one of the transmitting and receiving steps being performed at least in part by use of the first antenna.

In another aspect, the present invention is an apparatus for magnetic resonance imaging. The apparatus preferably comprises a magnet defining a patient-receiving space and having a static magnetic field with a field vector in a substantially horizontal direction and a patient support having a support surface for a human body. The patient support is preferably positioned within said patient-receiving space and is preferably pivotable about a horizontal pivot axis. The apparatus further desirably includes a quadrature coil antenna arrangement for receiving a signal from a patient disposed within the receiving space. The quadrature coil antenna preferably includes a first antenna having a first coil vector and a second antenna having a second coil vector, the first coil vector and said second coil vector being substantially transverse to said static magnetic field vector. The static magnetic field vector is preferably oriented substantially transverse to the long axis of a patient disposed within the patient-receiving space.

In accordance with this aspect of the present invention, the first antenna and the second antenna each comprise a coil antenna configured in a butterfly geometry.

Further in accordance with this aspect of the present invention, the first antenna and the second antenna are desirably housed in a planar structure. Further still, the planar structure comprises a quadrature surface coil that is circularly polarized in a plane perpendicular to said magnetic field axis. In addition, the first and second coil vectors are preferably transverse to each other. It is further desirably if the planar structure can be adjusted along a lengthwise direction of the patient support surface perpendicular to the magnetic field axis.

In another aspect the present invention is a magnetic resonance imaging apparatus comprising a stationary magnet having a pair of elements spaced apart from one another along a horizontal axis and a patient-receiving space between the elements. The horizontal axis is preferably substantially transverse to the long axis of a patient disposed within the patient-receiving space on a bed pivotable about an horizontal axis and the magnet is preferably operable to direct flux between said elements through said patient-receiving space.

## 5

In accordance with this aspect of the present invention, the apparatus further desirably comprises a quadrature coil antenna arrangement for receiving a signal from a body disposed within the patient-receiving space, the quadrature coil antenna including a first antenna having a first coil vector and a second antenna having a second coil vector, the first coil vector and the second coil vector being oriented substantially transverse to each other. In addition, the quadrature coil antenna arrangement is preferably housed in a planar structure having a planar surface in a plane perpendicular to the magnetic field axis.

In another aspect the present invention comprises a system for magnetic resonance imaging comprising a magnet defining a patient-receiving space and having a static magnetic field with a field vector in a substantially horizontal direction; a patient support having a surface capable of supporting a human body, the patient support being positioned within the patient-receiving space and being pivotable about a horizontal pivot axis parallel to the static magnetic field vector; and a quadrature coil antenna arrangement for receiving magnetic resonance signals from a patient disposed within the receiving space adjacent the patient support surface, the quadrature coil antenna including a first antenna having a first coil vector and a second antenna having a second coil vector, the first coil vector and the second coil vector being transverse to the static magnetic field vector.

In accordance with this aspect of the present invention, the first antenna desirably comprises a loop coil antenna and the second antenna comprises a butterfly coil antenna. In addition, the planar structure preferably comprises a quadrature surface coil that is circularly polarized in a plane perpendicular to said magnetic field axis.

Further in accordance with this aspect of the present invention, the planar structure is preferably adjustable along a lengthwise direction of the bed's surface perpendicular to the magnetic field axis.

Further in accordance with this aspect of the present invention, the first antenna preferably comprises a coil antenna configured as loop coil and the second antenna preferably comprises an antenna configured as a butterfly coil.

In another aspect, the present invention is an apparatus for magnetic resonance imaging. The apparatus preferably comprises a magnet defining a patient-receiving space and having a static magnetic field with a field vector in a substantially horizontal direction; a patient support having a support surface for a human body, said patient support being positioned within said patient-receiving space and being pivotable about a horizontal pivot axis; and a quadrature coil antenna arrangement for receiving a signal from a patient disposed within said receiving space, said quadrature coil antenna including a first antenna having a first coil vector and a second antenna having a second coil vector, said first coil vector and said second coil vector being transverse to said static magnetic field vector, and wherein said static magnetic field vector is oriented substantially transverse to the long axis of a patient disposed within said patient-receiving space. In accordance with this aspect of the present invention, the first antenna comprises a loop coil antenna and the second antenna comprises a coil antenna configured in a butterfly geometry.

In accordance with this aspect of the present invention, the loop coil antenna magnetic sensitivity is aligned anterior to posterior with respect to an anatomy of a patient supported by the patient support. It may also be desirable if the butterfly coil antenna geometry is aligned inferior to posterior with respect to an anatomy of a patient supported by the patient support.

## 6

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustratively depicts a front view of an apparatus in accordance with an embodiment of the present invention;

FIG. 2 is a side view of the apparatus of FIG. 1;

FIG. 3 illustratively depicts a top view of an antenna in accordance with an aspect of the present invention;

FIG. 4 is an edge view of the antenna of FIG. 3;

FIG. 5 is a side view of the apparatus of FIG. 1 with the patient depicted in a horizontal position;

FIG. 6 illustratively depicts a perspective view of first and second antennas in accordance with an aspect of the present invention;

FIG. 6A illustratively depicts a perspective view of first and second antennas in accordance with a further aspect of the present invention;

FIG. 7 schematically illustrates a saddle coil antenna in accordance with another aspect of the present invention;

FIG. 8 illustratively depicts a patient support apparatus in accordance with another aspect of the present invention;

FIG. 9 illustrates an embodiment of a quadrature coil antenna having solenoidal coil antenna and a planar coil antenna;

FIG. 9A illustrates another embodiment of a quadrature coil antenna having solenoidal coil antenna and a planar coil antenna;

FIG. 10 illustrates another embodiment of a quadrature coil antenna having a solenoidal coil antenna and a saddle coil antenna;

FIG. 11A illustrates a schematic of yet another embodiment of a quadrature coil antenna having a solenoidal coil antenna and a saddle coil antenna;

FIG. 11B illustrates the quadrature coil antenna of FIG. 11A without the external casing so as to reveal the arrangement of the solenoidal and saddle coil antennas; and

FIG. 12 schematically illustrates another embodiment of resonance imaging magnet in accordance with the present invention.

FIG. 13 schematically illustrates an antenna assembly in accordance with an aspect of the present invention.

FIG. 14 schematically illustrates an antenna assembly in accordance with an aspect of the present invention.

## DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

Turning to FIGS. 1 and 2, there is illustrated an apparatus 1 according to one embodiment of the present invention. The apparatus 1 includes a static field magnet having a frame 10 including a pair of poles 12 spaced apart from one another along a horizontal pole axis 14. Frame 10 further includes flux conducting and return members that, in the particular embodiment illustrated, include a pair of sidewalls 16 and columns 18 extending between the sidewalls 16. The particular frame depicted in FIGS. 1 and 2 is generally in accordance with the aforementioned U.S. Pat. No. 6,677,753, (hereinafter "the '753 patent") although other configurations can be employed. The opposed poles define a patient-receiving space or gap 20 between them. The magnet further includes a source of magnetic flux adapted to direct into and out of the gap through poles 12 so as to form a static magnetic field having a field vector  $B_0$  in the horizontal direction, parallel to pole axis 14. In the particular embodiment illustrated, the flux source includes a pair of electromagnet coils 22 encircling poles 12. These coils may be superconductive or resistive

coils. Alternate flux sources such as coils disposed at other locations along the ferromagnetic frame and permanent magnets also may be employed.

The apparatus further includes a patient support assembly including a bed **24** defining an elongated patient supporting surface **26** having a lengthwise axis **25** and a platform **28** projecting from the supporting surface at a foot end of the bed. In addition, a seat may be mounted to supporting surface **26** to allow a patient to be positioned in a sitting position. The patient supporting assembly further includes a frame **30**. Bed **24** is pivotably mounted to the frame **30** for movement about a generally horizontal pivot axis **32**. Pivot axis **32** is substantially parallel to pole axis **14**. Bed **24** can pivot between an upright position in which the lengthwise direction over the bed extends generally vertically as seen in FIG. **2** and a fully horizontal position shown in FIG. **5**, in which the lengthwise direction of the bed **24** extends horizontally. As further described in the '753 patent, bed **24** also may be mounted for vertical motion relative to frame **30** and hence relative to the static field magnet **10**. Moreover, frame **30** can be mounted for horizontal movement relative to the static field magnet. Appropriate actuators and control devices (not shown) are provided for moving the bed and for moving support frame **30**.

The patient support assembly further includes a first antenna schematically depicted as a planar box **34** in FIGS. **1**, **2** and **5**. As best seen in FIGS. **3** and **4**, the antenna includes a plurality of coils **36** each including a winding extending in a loop. Each loop may be provided with a conventional coupling to a separate coaxial cable or other output line **37** for conveying signals to a receiver or receiving signals from a transmitter. Also, each loop may include a capacitor (not shown) in series and/or in parallel with the conductor forming the loop so as to define a resonant antenna circuit. The windings of each coil extend along a slightly curved coil surface seen in edge view in FIG. **4**. The term "coil surface" as used herein refers to an imaginary surface defined by the central axis of the conductors constituting the coil or antenna. For example, in the special case of a flat circular coil, the coil surface is the plane of the circle. Each coil surface defines a coil vector  $V_c$  normal to the coil surface itself. In the case of a curved coil surface, the coil vector of the coil surface as a whole can be taken as the integral of the normal vector to the coil surface over the entire area of the coil surface inside the coil.

The coils **36** are arrayed along the lengthwise axis **25** of bed **24** so that the coils overlap one another as shown in FIG. **3**. Such a mutual overlapping arrangement results in the coils having zero or nearly zero mutual inductance between the coils. Other arrangements which result in nearly zero mutual inductance include arranging the coils in a plane that may extend along an elongated patient support. Coil surfaces **36** extend generally parallel to the patient support surface **26** of bed **24**. Thus, the normal vectors of the coil surfaces are transverse to the patient support surface **26** of the bed. The coils may be formed on a thin, plate or sheet that overlies surface **26**. Alternatively, the coils **36** may be mounted inside of the bed so that the coils are disposed behind surface **26**. Conventional padding or covering layers (not shown) may be provided over the coils and/or support surface **26** for patient comfort.

The apparatus also includes, or is used in conjunction with, conventional field gradient coils (not shown) for applying magnetic field gradients within the patient-receiving space or gap **20** and an RF receiver and transmitter (not shown) for applying RF signals through one or more loops **36** of antenna **34** and for receiving magnetic resonance signals using one or

more loops **36**. Additionally, the apparatus includes conventional control and reconstruction equipment for actuating the various elements discussed above including the gradient coils and RF transmitter and receiver to elicit magnetic resonance signals and to convert the resulting magnetic resonance signals into a set of data defining an image of the patient. These elements may use the conventional techniques and principles of the magnetic resonance art and accordingly are not discussed in detail herein.

In a method according to a further aspect of the invention, a patient **P** is disposed on patient support **24** so that the patient's body overlies the support and the first antenna **34**. In the position illustrated, the posterior surface of the patient's torso is closely juxtaposed to the patient support and with the first antenna so that the patient's spine is adjacent to the first antenna. The anterior-posterior axis of the patient's body is parallel to the coil vector  $V_c$  of the first antenna coils. The coil vector  $V_c$  lies in a plane perpendicular to the pole axis **14**. Thus, regardless of whether it is in an upright position as seen in FIG. **2** or in a fully horizontal position as seen in FIG. **5**, or at any angle between these positions, the coil vector  $V_c$  of the first antenna is perpendicular to the static magnetic field  $B_0$  so that the coils of the first antenna can interact with the body tissue to excite the nuclei to receive magnetic resonance signals. This arrangement provides excellent signal-to-noise ratio. Any portion of the patient's spine can be imaged using any one or more of the coils **36A-36D** in the first antenna. Further, this arrangement is entirely non-claustrophobic. The patient need not be constrained by the coils of the first antenna at all and the patient need not even be aware of the presence of the antenna.

Stated another way, the patient support surface **26** of support **24** lies substantially in a plane parallel to the pole axis **14** and hence parallel to the field vector of the static field magnet. This orientation allows the use of coils having coil surfaces generally parallel to the support surface. This arrangement of the support surface is different from the relative orientation of support surface and pole axis in a conventional "open" static field magnet having a vertical pole axis and a bed defining a substantially horizontal support surface, with the plane of the support surface perpendicular to the pole axis.

The same arrangement can be employed for imaging the patient in a prone position or standing position with the anterior surface of the torso facing the patient support surface **26**. Also, this arrangement can be used with the patient in a sideways position, with his lateral axis (shoulder-to-shoulder axis), parallel to the coil vectors  $V_c$ . A similar arrangement can be used for imaging portions of the body other than the torso as, for example, the head or legs.

Turning now to FIG. **6**, there is shown a perspective view of first and second antennas in accordance with another embodiment of the present invention. As FIG. **6** shows, a generally solenoidal second antenna **150** including a plurality of coils or loop windings **152** is used in conjunction with a first antenna **34** (similar to that discussed above). Each coil **152** of the second antenna extends in a plane transverse to the axis **153** of the antenna, and thus defines a coil having a coil vector  $V_{c152}$  extending substantially parallel to the axis **153** of the solenoid and parallel to the coil vectors of the other coils. The solenoidal coils may be electrically coupled to one another using couplers (not shown) similar to those discussed above with reference to FIG. **3** or, preferably, may be electrically independent of one another. In any event, whether electrically coupled together or not, the solenoidal coils magnetically behave as one solenoidal coil, i.e., magnetic coupling is independent of electrical coupling. The first antenna **34'** is similar to the first antenna **34** discussed above with reference to FIG.

3. The patient is positioned on the patient supporting surface (not shown) so that the patient overlies the first antenna **34** and so that the coils of the second antenna **150** encircle the patient's body. Solenoidal antennas that can be mounted so as to encircle the body of the patient in a convenient manner are disclosed, for example, in U.S. Pat. No. 4,887,038, the disclosure of which is hereby incorporated by reference herein. In FIG. **6**, the patient and the second antenna **150** are depicted at a substantial distance above the first antenna **34'** for clarity of illustration. In practice, the patient's body is positioned as close as is practicable to the first antenna.

In this arrangement, the coil vectors  $V_{c152}$  of the second antenna are substantially perpendicular to the coil vectors  $V_{c34'}$  of the first antenna and the coil vectors of both antennas are substantially perpendicular to the pole axis **14** and to the static field vector  $B_0$ , so that signals may be transmitted and/or received by either or both the first and second antennas. For example, the RF signals used to excite the nuclei may be transmitted by the second antenna and received by the first antenna or vice versa. Here again, the patient support may be arranged with the long axis of the patient's torso or other body structure horizontal or vertical.

Further in accordance with another aspect of the present invention, the first antenna **34'** of FIG. **6** is replaced with a planar antenna of the type depicted in FIG. **6A**. In particular, first antenna **44** includes one or more planar coil antennas, illustratively depicted as coils **44<sub>1</sub>** through **44<sub>3</sub>**. Coils **44<sub>1</sub>** through **44<sub>3</sub>** each comprise one or more windings extending in a loop. Each coil, **44<sub>1</sub>** through **44<sub>3</sub>**, includes a coil surface as described hereinabove. In addition, each coil surface defines a coil vector  $V_{c44}$  normal to the coil surface. Although coils **44<sub>1</sub>** through **44<sub>3</sub>** do not overlap, as in the embodiment shown in FIGS. **3** and **4**, the use of a planar antenna of the type depicted in FIG. **6A** for first antenna **44** results in an improvement in the signal-to-noise ratio of up to  $\sqrt{2}$ .

In a further embodiment, schematically illustrated in FIG. **7**, the first antenna is a saddle coil having a pair of windings each including a pair of axial runs **A** and a pair of arcuate runs **R** at the ends of the axial runs. Such a saddle coil defines a pair of coil surfaces in the form of sectors of a cylindrical surface. The coil vector of such a coil is perpendicular to the axis of the cylindrical surface. The first antenna may be arranged so that one of the saddle windings is disposed adjacent to the patient supporting surface **26** whereas the other is disposed remote from the patient supporting surface so that the patient's body is disposed between the two coils. Also, the first antenna may include additional sets of windings similar to the single set discussed above in reference to FIGS. **3** and **4**. One set may be disposed adjacent the patient supporting surface whereas the other set may be disposed remote from the patient supporting surface, and the patient may be held between these two sets. A solenoidal coil similar to coil **150** discussed above can be used in conjunction with such a first antenna.

In a further variant, the patient support may have a K form other than an elongated bed. For example, as seen in FIG. **8**, the patient support includes a chair having a seat **223** projecting in a forward or horizontal plane and a back **224** projecting upwardly from the seat so that the seat is disposed forward of the back. The back defines a first patient support surface **226** extending generally in a vertical plane whereas the seat defines a second patient support surface **227** extending generally in a horizontal plane. The seat is mounted in the patient-receiving space of a horizontal field magnet as discussed above. A first antenna **234** extends in or on the back so that it is closely juxtaposed with the first support surface **226**. The first antenna has one or more coils with coil vectors  $V_{c234}$ . A second antenna **235** extends in or on seat **223** so that it is

closely juxtaposed with the second support surface **227**. The second antenna **235** includes one or more coils with a coil vector  $V_{c235}$ . Both of these coil vectors are transverse to pole axis **214** and, therefore, both antennas can interact with atomic nuclei in the subject's body. The seat can be supported for pivoting motion and/or for vertical or horizontal movement within the patient-receiving space as discussed above. Even if the seat is pivoted about a horizontal axis parallel to the pole axis, the coil axes of both antennas will remain perpendicular to the pole axis. Apparatus according to this embodiment can be used, for example, to image the spine of a patient in the seated position or to image the perineal region or to image other structures in the patient's body. In particular, the apparatus of FIG. **8** may be advantageously used to image the pelvic region of a patient, as described in commonly assigned U.S. Application No. 60/342,382, filed on Dec. 20, 2001, and commonly assigned non-provisional United States application of Damadian, et al., entitled "MRI Apparatus Including Planar RF Coil Provided in a Seat," filed on even date herewith, the disclosures of which are hereby incorporated by reference herein.

Further in accordance with this aspect of the present invention, the quadrature coil arrangement of FIG. **8** may be achieved in an alternative embodiment by using seat **223** in combination with a planar coil antenna. In particular, first antenna **234** may comprise a planar coil antenna enclosed in a box. The box may then be inserted between support surface **226** and the surface of the patient adjacent to support surface **226**, e.g., the patient's back. The second antenna **235** is positioned or arranged so that it is positioned adjacent to the second support surface **227** or the sitting patient. Such a modular arrangement provides for greater flexibility yet while allowing for better signal-to-noise ratio.

The seat and/or the back of a chair as described above with reference to FIG. **8** can be provided as a removable element which can be attached to an elongated, bed-like patient support of the type discussed with reference to FIG. **1**. The first and second antennas likewise may be built into these removable elements, or may be provided as separate elements. Methods for attaching and adjusting the seat if implemented as a removable element are disclosed in commonly assigned U.S. application Ser. No. 10/131,843 ("the '843 application"), the disclosure of which is hereby incorporated by reference in its entirety.

Until now the arrangement shown in FIG. **8** was not considered exemplary of a class of antenna or coil arrangements commonly referred to as "quadrature coils." In such an arrangement the coil vectors associated with each of the antennas have mutually perpendicular axes. However, in accordance with this aspect of the present invention, the arrangement of two planar coils as shown in FIG. **8** may be used in a quadrature coil arrangement. In particular, in FIG. **8** the coil vector  $V_{c234}$  of antenna **234** is shown as projecting in a generally horizontal direction whereas the coil vector  $V_{c235}$  of antenna **235** is shown as projecting in a generally vertical direction. In this way both coil vectors are transverse to each other while being at the same time, as previously noted, transverse to the horizontal magnetic field  $B_0$ , which is oriented parallel to pole axis **214**. As described hereinabove, other novel quadrature coil arrangements are achievable in accordance with this aspect of the present invention. A quadrature coil antenna arrangement advantageously improves the signal-to-noise ratio by a factor up to  $\sqrt{2}$ . As a practical matter, the quadrature coil arrangement reduces the measurement or MRI scanning time by approximately one-half. That is, a measurement that takes approximately two minutes using a quadrature coil antenna arrangement will

take approximately four minutes using another antenna arrangement. This improvement in performance translates into increased efficiency at MRI facilities.

The arrangement shown in FIG. 6 may also be used as a quadrature coil antenna arrangement. In particular, solenoidal or second antenna **150** has a coil vector  $V_{C152}$  extending substantially parallel to the axis **153** of the antenna **150**. The coil vector  $V_{C34'}$  of the first antenna **34'** is substantially perpendicular to the coil vector  $V_{C152}$  of the of the second antenna **150**. The coil vectors of both the first and second antennas,  $V_{C34'}$  and  $V_{C152}$ , respectively, are also substantially perpendicular to the static field vector  $B_0$ . As such, the first and second antennas form a quadrature coil arrangement when used to receive the magnetic resonance signals.

Turning now to FIG. 9, there is illustrated another embodiment of a quadrature coil arrangement. Quadrature coil antenna **300** includes a first antenna schematically depicted as a planar box **302**. The one or more coils of the first antenna **302** may be arranged along a planar surface as shown in FIG. 3 and as shown by broken lines **303** in FIG. 9. First antenna **302** defines a coil vector  $V_{C302}$  that projects in a direction substantially transverse to the planar surface and, when attached to bed **24**, transverse to the patient support surface **26** of the bed **24** (see FIGS. 1 and 2). Quadrature coil antenna **300** includes a second antenna **312** having solenoidal coil portions **314**, **316** and **318**. The coil vector  $V_{C312}$  of the second magnet **312** projects in a direction transverse to the first antenna coil vector  $V_{C302}$ . Both the first and second coil vectors,  $V_{C302}$  and  $V_{C312}$ , are perpendicular to static field vector  $B_0$  of a horizontal field magnet of the type shown in FIGS. 1 and 2. First antenna **302** augments the signal of the second antenna **312** at the depth of the spine, thereby improving the quality of scanned images for this region. The second antenna **312** augments the signal of the first antenna **302** as the distance from the top of the solenoidal coils **314**, **316** and **318** increases.

Solenoidal coil portions **314**, **316** and **318** and latches **322** and **328** form an integral detachable unit. As depicted, latches **322** and **324** and latches **328** and **330** form male-female pairs that divide the antenna **300** into a front section comprising latches **322** and **328** and solenoidal coil portions **314**, **316** and **318** and a bottom section comprising first antenna **302**, latch members **324** and **330**, locking knobs **340** and **342**, and solenoidal coil portions **344**, **346** and **348**. As such, the quadrature antenna **300** opens in the front by removal of the front section from the back section. Detachable front and bottom sections allow for interchangeable varying size front sections that can optimize the coil size to the patient. In addition, the exposed portion of the solenoidal coil, including the removable front section, comprises a grid-like or skeletonized structure, which results in weight reduction and minimizes claustrophobic patient responses. The front section of quadrature antenna **300** may be optionally left off to allow the first or planar antenna **302** to function as a stand-alone unit.

The quadrature antenna **302** incorporates positioning features that allow the user to attach the coil assembly to the bed **24** of FIGS. 1 and 2 and to vertically adjust the assembly along the bed to accommodate the patient's anatomy. In addition, the positioning features allow an operator to easily lock the coil assembly in place anywhere along the vertical axis of the bed and use the coil with the patient sitting, standing, recumbent or at any angle. Methods and structures for attaching, adjusting and locking an antenna to the bed are disclosed in the '843 application; the same methods and structures can be used to attach, adjust and lock any of the antenna assemblies or arrangements which are described herein.

In a method in accordance with a further aspect of the invention, the quadrature antenna **300** is attached to the

patient support **24**. A patient P is then disposed on the patient support such that the posterior surface of the patient's torso is closely juxtaposed to the patient support and with first antenna **302**. In this way the patient's spine is adjacent to the first antenna **302**. The front section of the antenna **300** is then latched into place. As such, the coil vector  $V_{C302}$  of the first antenna **302** is perpendicular to the static magnetic field vector  $B_0$  and to the support surface **26**. The coil vector  $V_{C312}$  of the second antenna **312** project in a direction parallel to lengthwise axis **25** while being perpendicular to static magnetic field vector  $B_0$ . Both antennas are thereby available to receive the magnetic resonance signals emitted from the atomic nuclei of the patient P.

In a further variant, the one or more coils **303** shown in FIG. 9 may be preferably oriented as shown in FIG. 9A. That is, the windings on one or more coils **303'** of the planar antenna **302'** of FIG. 9A comprise a phased array of two coupled overlapping loops. As shown, the overlap is oriented longitudinally along the patient's body, i.e., along the long axis of the patient's body. In this way, the proximity of the coil to a patient's spinal cord is accomplished, resulting in improved signal-to-noise ratio in the area of interest.

Turning now to FIG. 10, which schematically illustrates another embodiment of a quadrature coil antenna **400** in accordance with the present invention. Quadrature coil antenna **400** comprises receiving solenoidal coil antenna **404** which comprises coils **412** and **414**. Solenoidal coil antenna **404** is combined in quadrature mode with a saddle coil **424**. One portion of saddle coil antenna **424** comprises the U-shaped coil **426** and an arcuate run  $R_1$  transverse to the U-shaped coil **426** along member **430** as shown. Another portion of saddle coil antenna **424** is formed by the U-shaped coil **428** and arcuate run  $R_2$ , which runs transverse to the U-shaped coil **428** along member **430**. As shown, the saddle coil **424** is rotated 90 degrees so that its magnetic sensitivity is now aligned posterior to anterior with respect to a patient's anatomy. The coil vector  $V_{C424}$  of the saddle coil antenna **424** projects in a direction perpendicular to static magnetic field vector  $B_0$  and to the coil vector  $V_{C404}$  of solenoidal coil antenna **404** when used in the apparatus **1** of FIGS. 1 and 2. The coil vector  $V_{C404}$  of coil antenna **404** also projects in a direction substantially perpendicular to static magnetic field vector  $B_0$ .

The solenoidal antenna **404** is mounted onto a base **440**. The U-shaped coils of the saddle coil antenna **424** are integrated with the solenoidal antenna **404** to form a skeletal structure into which a patient's head may be inserted. The antenna **400** may be attached to the patient bed **24** via the base **440** and vertically adjusted along the bed to adjust the patient's anatomy. The antenna may also be easily locked into place anywhere along the vertical axis **25** of the bed **24**. The attachment, vertical adjustment and locking features are described in the '843 application. The saddle coil **424** enhances the sensitivity in the direction of the static magnetic field vector ( $B_0$  in FIGS. 1 and 2). In addition, the patient's line of sight remains unobstructed during a scan which reduces claustrophobic effects. The antenna **400** also includes a convenient and effective left-right and front-back immobilization system comprising adjustable clamps **450**, which is adjustable to the patient's anatomy.

In a further variant, the coil **400** may be implemented so as to include separable portions or with a flip-up like visor. In such an embodiment, electrical continuity may be maintained by including male-female sockets at the separation points.

In accordance with an additional method aspect of the present invention, quadrature coil antenna **400** is attached to the patient support **24**. A patient P is then disposed on the

patient support such that the patient's head is placed in the quadrature coil antenna **400**. Stabilizing clamps **450** may then be used to stabilize the patient's head. In this position, the coil vector  $V_{C404}$  of solenoidal coil antenna **404** projects in a direction parallel to lengthwise axis **25** and perpendicular to static field vector  $B_0$ . Saddle coil vector  $V_{C424}$  projects in a direction transverse to the support surface **26** and is also perpendicular to static field vector  $B_0$ . The patient's head may then be scanned with the patient support rotated or positioned in the many orientations discussed hereinabove. In particular, the adjustable clamps **450** provide stabilization with the patient rotated or titled in many positions previously discussed hereinabove in relation to FIGS. **1**, **2** and **5**.

Turning now to FIG. **11A**, there is illustrated a schematic of yet another quadrature coil antenna in accordance with an aspect of the present invention. Quadrature coil **500** is used for preferably imaging a patient's knee. As can be best seen from FIG. **11B**, quadrature coil **500** comprises a solenoidal-receiver coil **504** and a saddle-style receiver coil **508**. Solenoidal-coil receiver **504** comprises individual coils **504<sub>1</sub>**, **504<sub>2</sub>**, **504<sub>3</sub>** and **504<sub>4</sub>**. In particular, coils **504<sub>4</sub>** and **504<sub>3</sub>** form one solenoidal loop and coils **504<sub>1</sub>** and **504<sub>2</sub>** form another solenoidal loop. This solenoidal coil vector  $V_{C504}$  projects in a direction perpendicular to static field vector  $B_0$  when used in the apparatus **1** of FIGS. **1** and **2**. Saddle coil **508** comprises coil members **508<sub>1</sub>**, **508<sub>2</sub>**, **508<sub>3</sub>** and **508<sub>4</sub>**. Coil members **508<sub>1</sub>** and **508<sub>2</sub>** form a continuous loop comprising the upper portion of saddle coil **508**. Saddle coil members **508<sub>3</sub>** and **508<sub>4</sub>** form another loop comprising the lower portion of saddle coil receiver **508**. A saddle-coil vector  $V_{C508}$  projects in a direction perpendicular to static-magnetic field  $V_0$  when used in the apparatus **1** of FIGS. **1** and **2**. As FIG. **11B** shows, the windings of the solenoidal coils **504** encircle the windings of the saddle coils **508**.

In a first embodiment, knee-coil **500** may be implemented to open at latch members **518** and **520** (see FIG. **11A**.) A patient's knee **K** is then positioned within knee-coil **500** and the antenna assembly is completed by latching members **518** and **520**. In accordance with this first embodiment of knee coil **500**, electrical continuity can be maintained by including male-female members where solenoidal coils **504<sub>1</sub>** through **504<sub>4</sub>** need to be mated. The patient is then placed on support surface **26**. Support surface **26** or table **24** is then moved into position so that the patient's knee is within the static-magnetic field. Imaging then proceeds. In accordance with the present invention, such imaging may proceed under a weight bearing or non-weight bearing condition.

In accordance with a further variant, knee coil **500** may be implemented as a single integrated unit, which is then pulled over a patient's foot up to the patient's knee. In addition, the knee coil **500** may also be implemented such that it swings open at either latch **518** or **520**.

In addition to the magnet structure shown in FIGS. **1**, **2** and **5**, the quadrature coil arrangement described hereinabove may also be used in a magnet structure **1000**, as shown in FIG. **12**. The magnet **1000** includes a stationary magnet having a pair of elements, **1010** and **1020**, spaced apart from one another along horizontal axis **X**. A magnetic air gap between elements **1010** and **1020** define a patient-receiving space **1035**. Each of the elements **1010** and **1020** include one or more solenoidal superconducting coils **1040**. The coils **1040** are operative to direct magnetic flux between the elements **1010** and **1020** so as to establish a horizontal static magnetic field  $B_0$ . The elements **1010** and **1020** are mounted to structural support member **1045**, which maintains the gap between the elements. The magnet **1000** may optionally include ferromagnetic poles **1051**. However, poles **1051** may be elimi-

nated and the magnet **1000** may nonetheless operate in accordance with the present invention.

In accordance with the embodiment shown in FIG. **12**, a patient **P** may be positioned within the patient-receiving space **1035** such that the long axis **1055** of the patient's body is transverse to static magnetic  $B_0$ . The patient may be positioned in the sitting or standing position in accordance with the requirements associated with the medical procedure. In addition, the patient may also be fitted with any of the quadrature coil antennas described in detail hereinabove so that magnetic resonance scanning may be advantageously performed. In particular, the signal-to-noise ratios improvement of up to  $\sqrt{2}$  may be achieved in accordance with this embodiment.

Turning now to FIG. **13**, there is shown a quadrature surface coil antenna **1300** in accordance with a further aspect of the present invention. The antenna **1300** includes a pair of substantially flat butterfly receiver coils **1304**, **1306** that are arranged in quadrature mode as shown. In particular, a first coil vector  $V_{1304}$  of coil **1304** is oriented parallel to a plane in which the receiver coil **1304** lies. A second coil vector  $V_{1306}$  of coil **1306** is also oriented perpendicular to first coil vector  $V_{1304}$  and parallel to a plane in which receiver coil **1306** lies. In the preferred embodiment, the coils **1304**, **1306** are mounted to a base **1310** that forms a planar structure or box for housing the quadrature surface coil antenna **1300**. The planar structure or box is shown without a top that is attachable to the base **1310** so as to conveniently reveal the arrangement of the butterfly coils **1304**, **1306**. In accordance with this aspect of the present invention, the coils vectors are oriented parallel to surface of the planar structure or box.

As shown, each coil **1304**, **1306** includes a pair of tap off points **1314<sub>1,2</sub>**, **1316<sub>1,2</sub>** at which circuitry necessary to the operation of the coils may be located. Such circuitry serve to decouple the individual antennas, define a resonant antenna circuit and output the magnetic resonance signals received (e.g., see output port **1320**).

The quadrature surface coil antenna **1300** may be used in the apparatus **1** shown in FIG. **2** by positioning the structure housing the antenna **1300** parallel to surface of the poles **12**. In particular, a side of the structure or planar box **1310** is positioned adjacent to the patient supporting surface **26** such that each of the coil vectors  $V_{1304}$ ,  $V_{1306}$  are substantially orthogonal or perpendicular to the horizontal pole axis **14** and the direction of the static magnetic field  $B_0$ . Since the geometry of the butterfly coils allow for 360° of freedom in positioning the structure or box **1310** in any plane parallel with the pole surfaces, the antenna assembly **1300** can be rotated into any orientation in such a plane to complement the patient anatomy. The magnetic sensitivity of the coils can be rotated from posterior/anterior to inferior/superior and any point in between that suits the anatomical surfaces. The antenna **1300** may be useful in imaging the spine or other portions of a patient's anatomy.

In addition, the quadrature coil antenna **1300** is advantageously circularly polarized in a plane perpendicular to the direction of the static magnetic field  $B_0$ . The antenna **1300** desirably produces it strongest magnetic sensitivity at the intersection of the butterfly elements. Therefore, the symmetry of the arrangement produces an even circular illumination of the anatomy with signal-to-noise that is approximately 40% greater than a single butterfly coil. As discussed, the antenna **1300** is preferably flat and is positionable parallel to the surface of the poles of the magnet. However, the antenna may be similarly used even in a magnet without distinct poles as long as the coil vectors are oriented perpendicular to the direction of the static magnetic field. As such, the quadrature



15

surface **1300** is also adaptable to imaging in a vertical field system with the coil surface parallel to the patient support surface.

Turning now to FIG. **14**, there is shown a quadrature planar coil antenna assembly **1400** in accordance with an additional aspect of the present invention. As shown, the assembly **1400** includes a loop coil antenna **1402** and a butterfly coil antenna **1406** mounted to a base or support **1412** using a plurality of mounting members **1414**. As shown, each mounting member conveniently includes an opening large enough to accommodate a portion of the coil and secures the coil to base **1412** via various mounting screws. The loop coil antenna **1402** includes a coil vector  $V_{1402}$  perpendicular to the surface of the base **1412**. The butterfly coil **1406** includes a coil vector  $V_{1406}$  that is parallel to the surface of the base **1412**. The assembly also includes circuitry **1420** (shown not connected) for outputting magnetic resonance signals received by the coils. Such circuitry serves to decouple the individual antennas, define a resonant antenna circuit and output the magnetic resonance signals received by the antenna coils.

In accordance with this aspect of the present invention, the planar coil assembly **1400** may be used with the system of FIGS. **1** and **2** with a patient oriented in any position between an upright and recumbent position as long as the coil vectors  $V_{1402}$ ,  $V_{1406}$  are perpendicular to the static magnetic field  $B_0$ . In particular, while the loop coil's magnetic sensitivity is aligned posterior to anterior with respect to the patient's anatomy, the butterfly coil's magnetic sensitivity is aligned inferior to superior or vice versa. In accordance with an aspect of the present invention, a patient may be positioned in an upright position, as shown in FIG. **2** for example, with the antenna assembly **1400** between a surface of the patient's anatomy and the surface of the patient support device **24**. Although FIGS. **1** and **2** depict the antenna as being adjacent to the posterior surface of the patient **P**, the antenna may be positioned adjacent to the anterior surface of the patient. The antenna **1400** may be vertically adjusted along the support surface **26** to allow for imaging of the spine, heart, or other areas of the torso. In addition, the antenna may be positioned as shown in FIG. **8** so as to allow a patient to sit on the antenna so that images of the lower abdomen, e.g., pelvic region or prostate, can be obtained.

In accordance with this aspect of the present invention, the loop coil typically augments the signal of the butterfly coil where the butterfly coil tends to be weakest. In addition, the butterfly coil typically augments the signal received by the loop coil where the loop coil tends to be weakest. The antenna coil **1400** is advantageously circularly polarized in a plane perpendicular to the horizontal field  $B_0$  of the magnet. Therefore, the antenna coil **1400** may be used in any magnet geometry where the antenna coil is circularly polarized in a plane perpendicular to the horizontal field of the magnet.

Although the invention herein has been described with reference to particular embodiments, it is to be understood that these embodiments are merely illustrative of the principles and applications of the present invention. It is therefore

16

to be understood that numerous modifications may be made to the illustrative embodiments and that other arrangements may be devised without departing from the spirit and scope of the present invention as defined by the appended claims. In particular, quadrature coils may be designed for many more parts of the human anatomy, e.g., the ankle, wrist, shoulder, neck, foot, breast, etc., that would provide improved signal-to-noise ratio performance.

The invention claimed is:

1. Apparatus for magnetic resonance imaging, comprising:
  - a magnet defining a patient-receiving space and having a static magnetic field with a field vector in a substantially horizontal direction;
  - a patient support having a support surface for a human body, said patient support being positioned within said patient-receiving space and being pivotable about a horizontal pivot axis; and
  - a quadrature coil antenna arrangement for receiving a signal from a patient disposed within said receiving space, said quadrature coil antenna including a first antenna having a first coil vector and a second antenna having a second coil vector, said first coil vector and said second coil vector being transverse to said static magnetic field vector, and wherein said static magnetic field vector is oriented substantially transverse to the long axis of a patient disposed within said patient-receiving space, wherein said first antenna and said second antenna comprise coil antennas configured in a dual butterfly geometry housed in a planar structure and wherein the position of the planar structure can be adjusted along a lengthwise direction of the patient support surface perpendicular to said magnetic field axis.
2. The apparatus as claimed in claim 1, wherein said first and second coil vectors are transverse to each other.
3. The apparatus as claimed in claim 2, wherein said planar structure is oriented such that its surface lies in a plane perpendicular to said magnetic field axis.
4. The apparatus as claimed in claim 2, wherein said planar structure comprises a quadrature surface coil that is circularly polarized in a plane perpendicular to said magnetic field axis.
5. The apparatus as claimed in claim 1, further comprising an elevator for raising and lowering said patient support relative to said magnet while the patient support is holding the patient in an upright orientation so as to position any part of the patient within said patient-receiving space.
6. The apparatus as claimed in claim 1, wherein said first antenna and said second antenna are substantially flat.
7. The apparatus as claimed in claim 1, wherein said first coil vector is oriented parallel to a plane in which said first antenna lies and said second coil vector is oriented perpendicular to said first coil vector and parallel to a plane in which said second antenna lies.
8. The apparatus as claimed in claim 1, wherein said first coil vector and said second coil vector are oriented parallel to said planar structure.

\* \* \* \* \*

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**


PATENT NO. : 7,701,209 B1  
APPLICATION NO. : 10/998395  
DATED : April 20, 2010  
INVENTOR(S) : Charles A. Green

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

- Column 2, line 68, "patient can" should read --patient, can--.
- Column 3, line 41, "second coil vector" should read --second coil vectors--.
- Column 3, line 53, "antennas being" should read --antennas are--.
- Column 4, line 14, "method for" should read --a method for--.
- Column 4, line 65, "about an" should read --about a--.
- Column 5, line 39, "as loop" should read --as a loop--.
- Column 6, line 23, "having solenoidal" should read --having a solenoidal--.
- Column 6, line 26, "having solenoidal" should read --having a solenoidal--.
- Column 6, line 37, "embodiment of" should read --embodiment of a--.
- Column 7, line 56, "thin, plate" should read --thin plate--.
- Column 11, line 9, "of the of the second" should read --of the second--.
- Column 12, line 9, "312 project" should read --312 projects--.
- Column 12, line 21, "resulting in" should read --resulting in an--.
- Column 13, line 60, "1020 include" should read --1020 includes--.
- Column 14, line 30, "the coils" should read --the coils'--.
- Column 14, line 43, "are substantially" should read --is substantially--.
- Column 14, line 46, "coils allow" should read --coils allows--.
- Column 14, line 58, "produces it" should read --produces its--.
- Column 15, line 51, "may used" should read --may be used--.
- Column 16, line 51, "a plan in" should read --a plane in--.

Signed and Sealed this  
Fourteenth Day of June, 2011

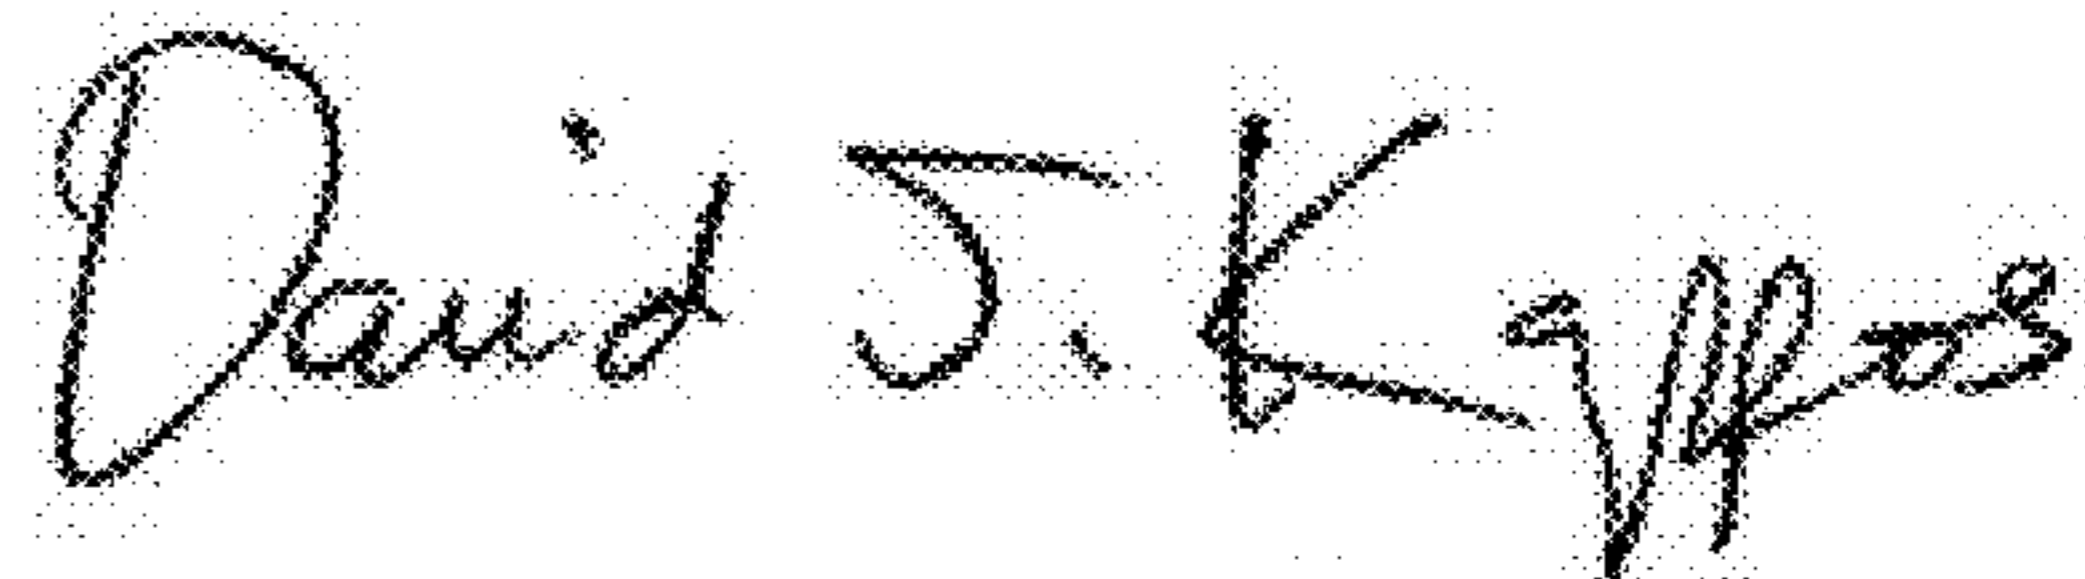

David J. Kappos  
*Director of the United States Patent and Trademark Office*