



US007842053B2

(12) **United States Patent**
Chanduszko et al.

(10) **Patent No.:** **US 7,842,053 B2**
(45) **Date of Patent:** **Nov. 30, 2010**

- (54) **DOUBLE COIL OCCLUDER**
- (75) Inventors: **Andrzej J. Chanduszko**, Chandler, AZ (US); **David R. Widomski**, Wakefield, MA (US)
- (73) Assignee: **NMT Medical, Inc.**, Boston, MA (US)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 314 days.

4,693,249 A	9/1987	Schenck et al.
4,696,300 A	9/1987	Anderson
4,710,181 A	12/1987	Fuqua
4,710,192 A	12/1987	Liotta et al.
4,738,666 A	4/1988	Fuqua
4,836,204 A	6/1989	Landymore et al.
4,840,623 A	6/1989	Quackenbush

(Continued)

(21) Appl. No.: **11/093,348**

FOREIGN PATENT DOCUMENTS

(22) Filed: **Mar. 30, 2005**

DE 9413645 U1 10/1994

(65) **Prior Publication Data**

US 2005/0251154 A1 Nov. 10, 2005

(Continued)

Related U.S. Application Data

(60) Provisional application No. 60/568,526, filed on May 6, 2004.

OTHER PUBLICATIONS

(51) **Int. Cl.**
A61B 17/08 (2006.01)

Applied Fibre Science, F. Happey, Ed. Chapter 8, E. Atkins, Academic Press, New York 1979.

(52) **U.S. Cl.** **606/157**

(Continued)

(58) **Field of Classification Search** 606/215, 606/139, 151, 157, 159, 213, 232; 623/3.1
See application file for complete search history.

Primary Examiner—(Jackie) Tan-Uyen T Ho
Assistant Examiner—Gregory Anderson
(74) *Attorney, Agent, or Firm*—Helen S. Liu

(56) **References Cited**


(57) **ABSTRACT**

U.S. PATENT DOCUMENTS

3,344,048 A	9/1967	Kobetz et al.
3,824,631 A	7/1974	Burstein et al.
3,874,388 A	4/1975	King et al.
3,875,648 A	4/1975	Bone
3,924,631 A	12/1975	Mancusi, Jr.
4,006,747 A	2/1977	Kronenthal et al.
4,007,743 A	2/1977	Blake
4,149,327 A	4/1979	Hammer et al.
4,425,908 A	1/1984	Simon
4,610,674 A	9/1986	Suzuki et al.
4,626,245 A	12/1986	Weinstein

An occluder that has a coil on one or both sides of a medical defect, particularly a septal defect such as a patent foramen ovale (PFO). Each coil can be formed as a tube that is hollow, with or without a closed end. The tube can be delivered over a wire. For occluding a PFO, the coils can be designed to provide a compressive force to one or both of septum primum and septum secundum.

25 Claims, 14 Drawing Sheets

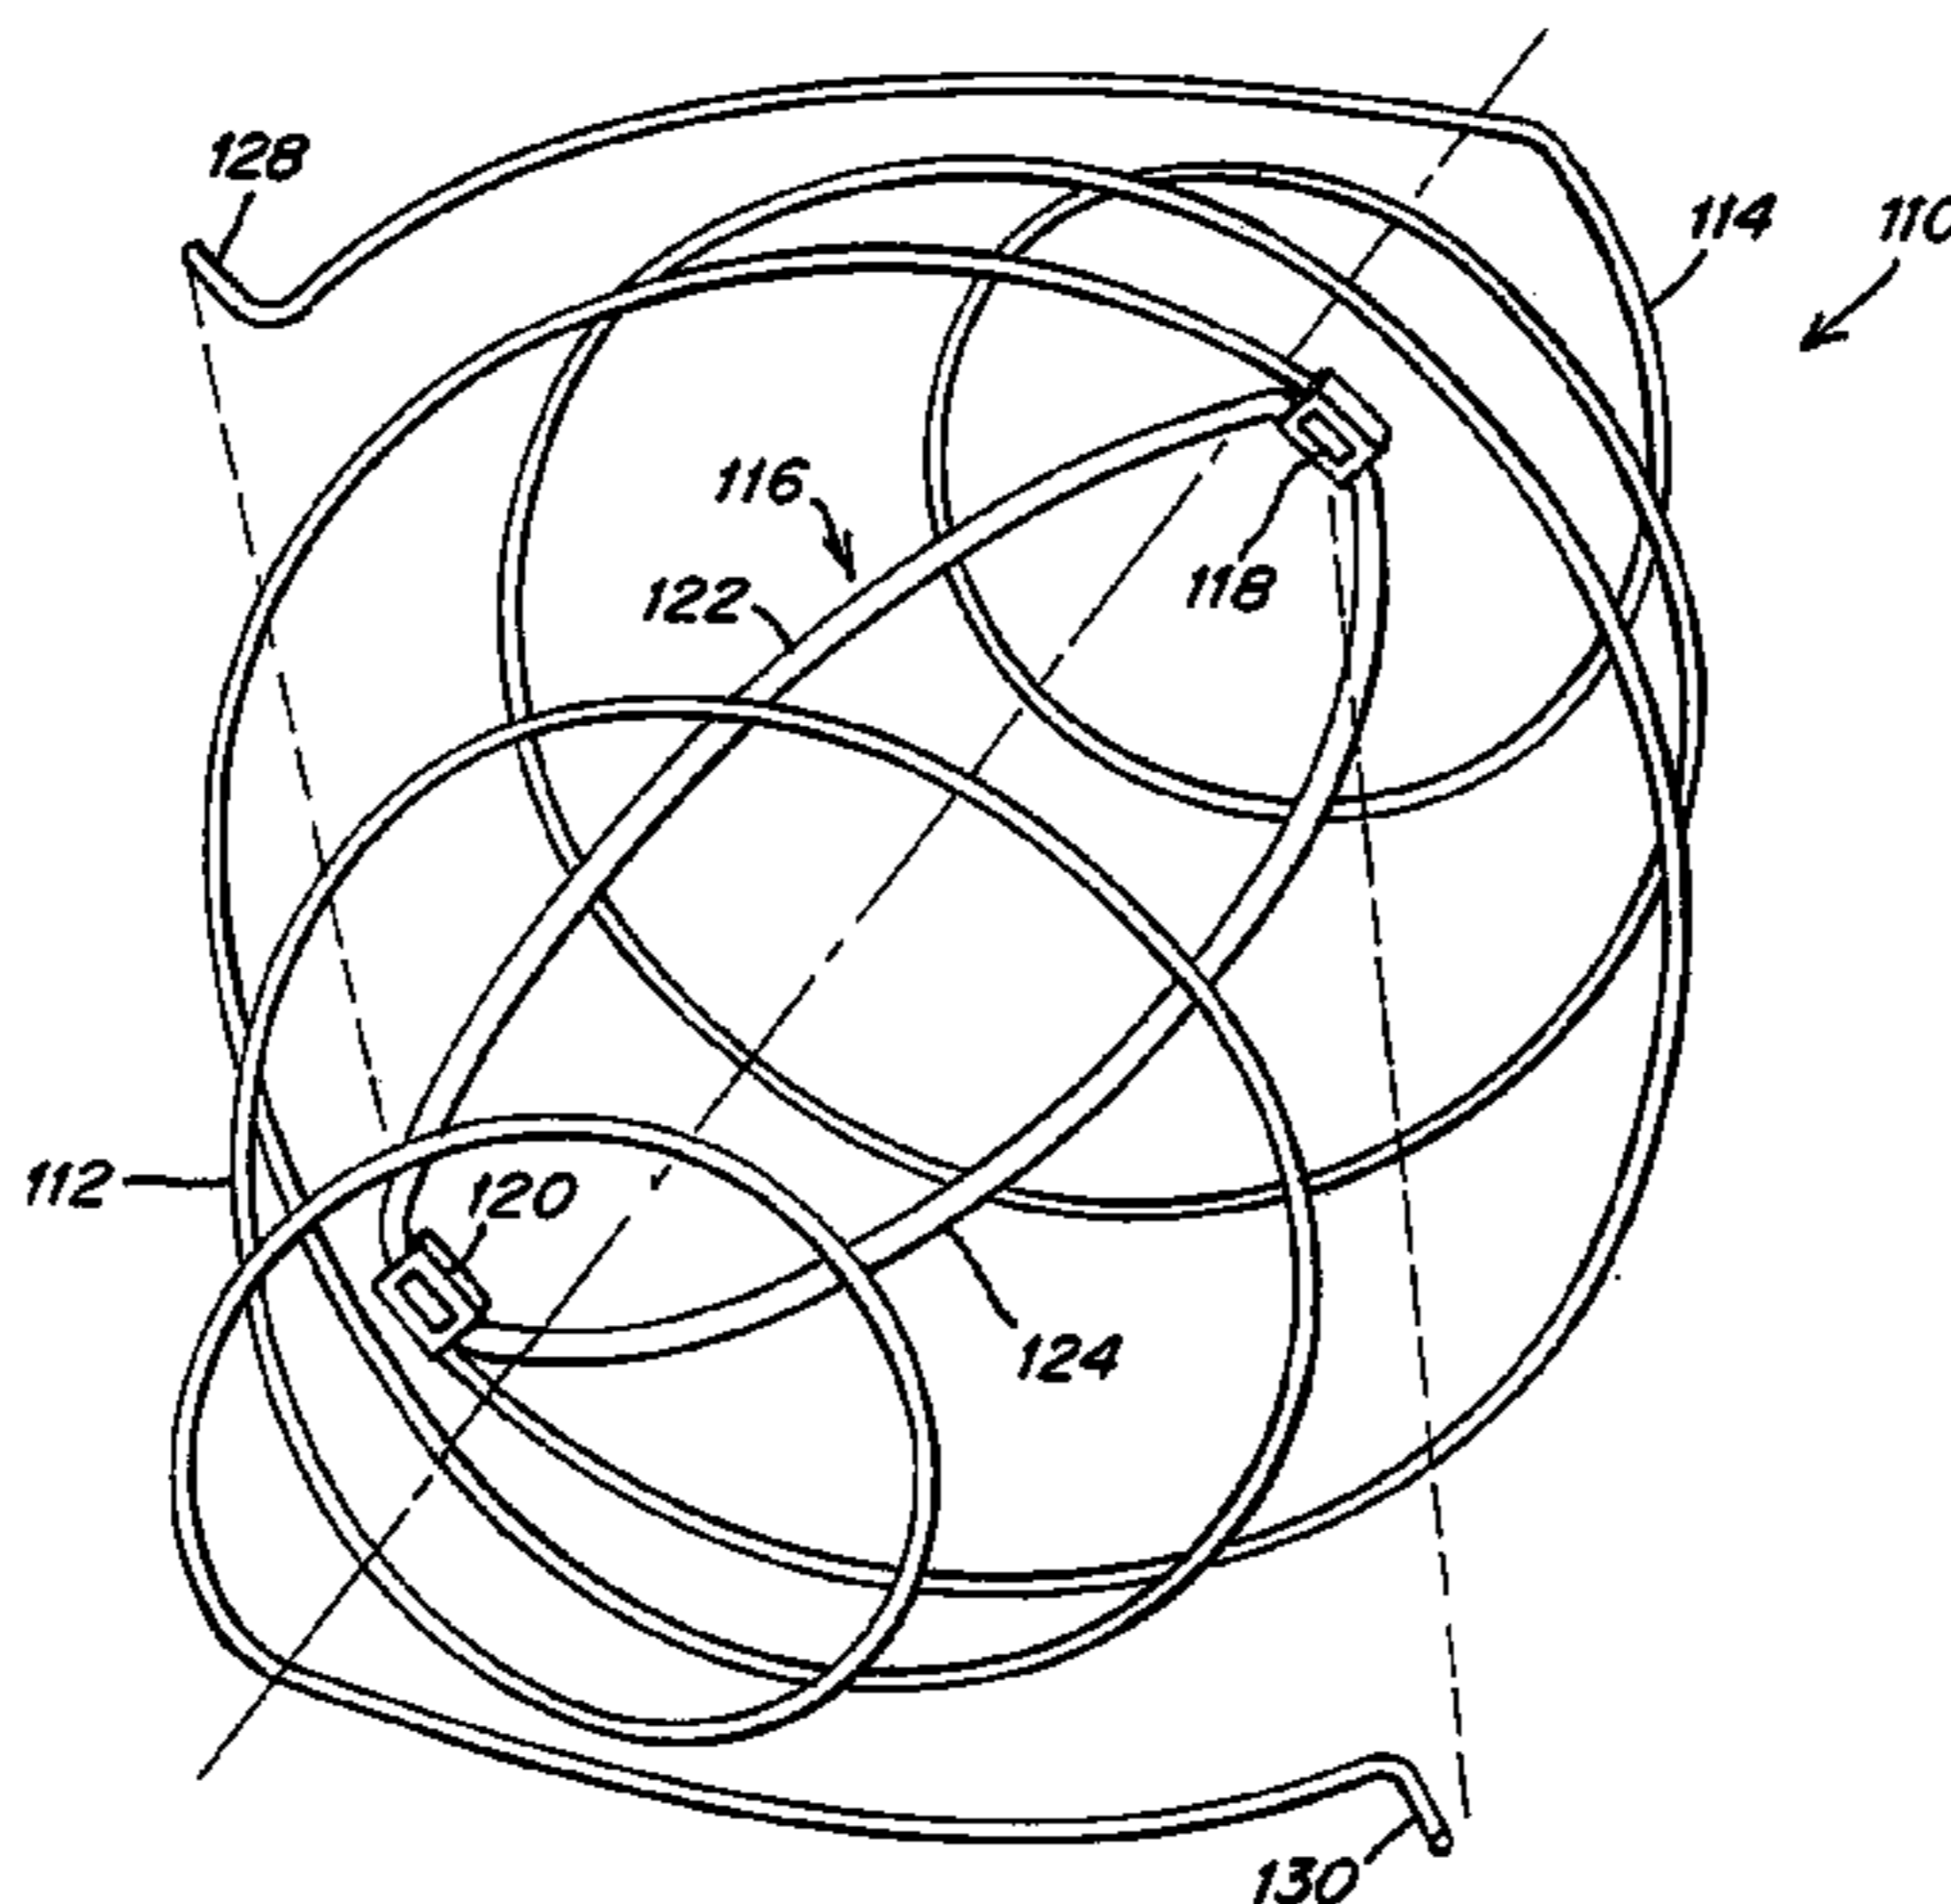

U.S. PATENT DOCUMENTS					
			5,725,552 A	3/1998	Kotula et al.
			5,733,294 A	3/1998	Forber et al.
			5,733,337 A	3/1998	Carr, Jr. et al.
			5,741,297 A	4/1998	Simon
			5,772,641 A	6/1998	Wilson
			5,776,162 A	7/1998	Kleshinski
			5,776,183 A	7/1998	Kanesaka et al.
			5,797,960 A	8/1998	Stevens et al.
			5,800,516 A	9/1998	Fine et al.
			5,810,884 A	9/1998	Kim
			5,820,594 A	10/1998	Fontirroche et al.
			5,823,956 A	10/1998	Roth et al.
			5,829,447 A	11/1998	Stevens et al.
			5,853,420 A	12/1998	Chevillon et al.
			5,853,422 A	12/1998	Huebsch et al.
			5,855,614 A	1/1999	Stevens et al.
			5,861,003 A	1/1999	Latson et al.
			5,865,791 A	2/1999	Whayne et al.
			5,879,366 A	3/1999	Shaw et al.
			5,893,856 A	4/1999	Jacob et al.
			5,902,287 A	5/1999	Martin
			5,902,319 A	5/1999	Daley
			5,904,703 A	5/1999	Gilson
			5,919,200 A	7/1999	Stambaugh et al.
			5,924,424 A	7/1999	Stevens et al.
			5,928,250 A	7/1999	Koike et al.
			5,944,691 A	8/1999	Querns et al.
			5,944,738 A	8/1999	Amplatz et al.
			5,955,110 A	9/1999	Patel et al.
			5,976,174 A	11/1999	Ruiz
			5,980,505 A	11/1999	Wilson
			5,989,268 A	11/1999	Pugsley, Jr. et al.
			5,993,475 A	11/1999	Lin et al.
			5,993,844 A	11/1999	Abraham et al.
			5,997,575 A	12/1999	Whitson et al.
			6,010,517 A	1/2000	Baccaro
			6,019,753 A	2/2000	Pagan
			6,024,756 A	2/2000	Huebsch et al.
			6,027,519 A	2/2000	Stanford
			6,030,007 A	2/2000	Bassily et al.
			6,056,760 A	5/2000	Koike et al.
			6,071,998 A	6/2000	Muller et al.
			6,077,291 A	6/2000	Das
			6,077,880 A	6/2000	Castillo et al.
			6,079,414 A	6/2000	Roth
			6,080,182 A	6/2000	Shaw et al.
			6,096,347 A	8/2000	Geddes et al.
			6,106,913 A	8/2000	Scardino et al.
			6,113,609 A	9/2000	Adams
			6,117,159 A	9/2000	Huebsch et al.
			6,126,686 A	10/2000	Badylak et al.
			6,132,438 A	10/2000	Fleischman et al.
			6,143,037 A	11/2000	Goldstein et al.
			6,152,144 A	11/2000	Lesh et al.
			6,165,183 A	12/2000	Kuehn et al.
			6,165,204 A	12/2000	Levinson et al.
			6,168,588 B1	1/2001	Wilson
			6,171,329 B1 *	1/2001	Shaw et al. 606/213
			6,174,322 B1	1/2001	Schneidt et al.
			6,174,330 B1	1/2001	Stinson
			6,183,443 B1	2/2001	Kratoska et al.
			6,187,039 B1	2/2001	Hiles et al.
			6,190,353 B1	2/2001	Makower et al.
			6,190,357 B1	2/2001	Ferrari et al.
			6,197,016 B1	3/2001	Fourkas et al.
			6,199,262 B1	3/2001	Martin
			6,206,895 B1	3/2001	Levinson
			6,206,907 B1	3/2001	Marino et al.
			6,214,029 B1	4/2001	Thill et al.
			6,217,590 B1	4/2001	Levinson
			6,221,092 B1	4/2001	Koike et al.
			6,227,139 B1	5/2001	Nguyen et al.
			6,228,097 B1	5/2001	Levinson et al.
4,902,508 A	2/1990	Badylak et al.			
4,915,107 A	4/1990	Rebuffat et al.			
4,917,089 A	4/1990	Sideris			
4,921,479 A	5/1990	Grayzel			
4,956,178 A	9/1990	Badylak et al.			
5,021,059 A	6/1991	Kensey et al.			
5,037,433 A	8/1991	Wilk et al.			
5,041,129 A	8/1991	Hayhurst et al.			
5,049,131 A	9/1991	Deuss			
5,078,736 A	1/1992	Behl			
5,106,913 A	4/1992	Yamaguchi et al.			
5,108,420 A	4/1992	Marks			
5,149,327 A	9/1992	Oshiyama			
5,163,131 A	11/1992	Row et al.			
5,167,363 A	12/1992	Adkinson et al.			
5,167,637 A	12/1992	Okada et al.			
5,171,259 A	12/1992	Inoue			
5,176,659 A	1/1993	Mancini			
5,192,301 A	3/1993	Kamiya et al.			
5,222,974 A	6/1993	Kensey et al.			
5,226,879 A	7/1993	Ensminger et al.			
5,236,440 A	8/1993	Hlavacek			
5,245,023 A	9/1993	Peoples et al.			
5,245,080 A	9/1993	Aubard et al.			
5,250,430 A	10/1993	Peoples et al.			
5,257,637 A	11/1993	El Gazayerli			
5,275,826 A	1/1994	Badylak et al.			
5,282,827 A	2/1994	Kensey et al.			
5,284,488 A	2/1994	Sideris			
5,304,184 A	4/1994	Hathaway et al.			
5,312,341 A	5/1994	Turi			
5,312,435 A	5/1994	Nash et al.			
5,316,262 A	5/1994	Koebler			
5,320,611 A	6/1994	Bonutti et al.			
5,334,217 A	8/1994	Das			
5,350,363 A	9/1994	Goode et al.			
5,354,308 A	10/1994	Simon et al.			
5,364,356 A	11/1994	Hofling			
5,411,481 A	5/1995	Allen et al.			
5,413,584 A	5/1995	Schulze			
5,417,699 A	5/1995	Klein et al.			
5,425,744 A	6/1995	Fagan et al.			
5,433,727 A	7/1995	Sideris			
5,451,235 A	9/1995	Lock et al.			
5,453,099 A	9/1995	Lee et al.			
5,478,353 A	12/1995	Yoon			
5,480,353 A	1/1996	Garza, Jr.			
5,480,424 A	1/1996	Cox			
5,486,193 A	1/1996	Bourne et al.			
5,507,811 A	4/1996	Koike et al.			
5,534,432 A	7/1996	Peoples et al.			
5,540,712 A	7/1996	Kleshinski et al.			
5,562,632 A	10/1996	Davila et al.			
5,577,299 A	11/1996	Thompson et al.			
5,601,571 A	2/1997	Moss			
5,603,703 A	2/1997	Elsberry et al.			
5,618,311 A	4/1997	Gryskiewicz			
5,620,461 A	4/1997	Muijs Van De Moer et al.			
5,626,599 A	5/1997	Bourne et al.			
5,634,936 A	6/1997	Linden et al.			
5,649,950 A	7/1997	Bourne et al.			
5,649,959 A	7/1997	Hannam et al.			
5,663,063 A	9/1997	Peoples et al.			
5,683,411 A	11/1997	Kavteladze et al.			
5,690,674 A	11/1997	Diaz			
5,693,085 A	12/1997	Buirge et al.			
5,702,421 A	12/1997	Schneidt			
5,709,707 A	1/1998	Lock et al.			
5,713,864 A	2/1998	Verkaart			
5,717,259 A	2/1998	Schexnayder			
5,720,754 A	2/1998	Middleman et al.			

US 7,842,053 B2

6,231,561 B1	5/2001	Frazier et al.	6,867,249 B2	3/2005	Lee et al.
6,245,080 B1	6/2001	Levinson	6,921,410 B2	7/2005	Porter
6,245,537 B1	6/2001	Williams et al.	2001/0010481 A1	8/2001	Blanc et al.
6,261,309 B1	7/2001	Urbanski	2001/0014800 A1	8/2001	Frazier et al.
6,265,333 B1	7/2001	Dzenis et al.	2001/0025132 A1	9/2001	Alferness et al.
6,270,515 B1	8/2001	Linden et al.	2001/0034537 A1	10/2001	Shaw et al.
6,277,138 B1	8/2001	Levinson et al.	2001/0034567 A1	10/2001	Allen et al.
6,277,139 B1	8/2001	Levinson et al.	2001/0037129 A1	11/2001	Thill
6,287,317 B1	9/2001	Makower et al.	2001/0039435 A1	11/2001	Roue et al.
6,290,674 B1	9/2001	Roue et al.	2001/0039436 A1	11/2001	Frazier et al.
6,299,635 B1	10/2001	Frantzen	2001/0041914 A1	11/2001	Frazier et al.
6,306,150 B1	10/2001	Levinson	2001/0041915 A1	11/2001	Roue et al.
6,306,424 B1	10/2001	Vyakarnam et al.	2001/0044639 A1	11/2001	Levinson
6,312,443 B1	11/2001	Stone	2001/0049492 A1	12/2001	Frazier et al.
6,312,446 B1	11/2001	Huebsch et al.	2002/0010481 A1*	1/2002	Jayaraman 606/151
6,315,791 B1	11/2001	Gingras et al.	2002/0019648 A1	2/2002	Akerfeldt et al.
6,316,262 B1	11/2001	Huisman et al.	2002/0022859 A1	2/2002	Hogendijk
6,319,263 B1	11/2001	Levinson	2002/0022860 A1	2/2002	Borillo et al.
6,322,548 B1	11/2001	Payne et al.	2002/0026208 A1	2/2002	Roe et al.
6,328,727 B1	12/2001	Frazier et al.	2002/0029048 A1	3/2002	Miller
6,334,872 B1	1/2002	Termin et al.	2002/0032459 A1	3/2002	Horzewski et al.
6,342,064 B1	1/2002	Koike et al.	2002/0032462 A1	3/2002	Houser et al.
6,344,048 B1	2/2002	Chin et al.	2002/0034259 A1	3/2002	Tada
6,344,049 B1	2/2002	Levinson et al.	2002/0035374 A1	3/2002	Borillo et al.
6,346,074 B1	2/2002	Roth	2002/0043307 A1	4/2002	Ishida et al.
6,348,041 B1	2/2002	Klint et al.	2002/0049457 A1	4/2002	Kaplan et al.
6,352,552 B1	3/2002	Levinson et al.	2002/0052572 A1	5/2002	Franco et al.
6,355,052 B1	3/2002	Neuss et al.	2002/0058989 A1	5/2002	Chen et al.
6,356,782 B1	3/2002	Sirimanne et al.	2002/0077555 A1	6/2002	Schwartz
6,358,238 B1	3/2002	Sherry	2002/0095174 A1	7/2002	Tsugita et al.
6,364,853 B1	4/2002	French et al.	2002/0096183 A1	7/2002	Stevens et al.
6,371,904 B1	4/2002	Sirimanne et al.	2002/0099389 A1	7/2002	Michler et al.
6,375,625 B1	4/2002	French et al.	2002/0099390 A1	7/2002	Kaplan et al.
6,375,671 B1	4/2002	Kobayashi et al.	2002/0099437 A1*	7/2002	Anson et al. 623/1.15
6,379,342 B1	4/2002	Levinson	2002/0103492 A1	8/2002	Kaplan et al.
6,379,368 B1	4/2002	Corcoran et al.	2002/0107531 A1	8/2002	Schreck et al.
6,387,104 B1	5/2002	Pugsley, Jr. et al.	2002/0111537 A1	8/2002	Taylor et al.
6,398,796 B2	6/2002	Levinson	2002/0111637 A1	8/2002	Kaplan et al.
6,402,772 B1	6/2002	Amplatz et al.	2002/0111647 A1	8/2002	Khairkhahan et al.
6,419,669 B1	7/2002	Frazier et al.	2002/0120323 A1	8/2002	Thompson et al.
6,426,145 B1	7/2002	Moroni	2002/0128680 A1	9/2002	Pavlovic
6,436,088 B2	8/2002	Frazier et al.	2002/0129819 A1	9/2002	Feldman et al.
6,440,152 B1	8/2002	Gainor et al.	2002/0164729 A1	11/2002	Skraly et al.
6,450,987 B1	9/2002	Kramer	2002/0169377 A1	11/2002	Khairkhahan et al.
6,460,749 B1	10/2002	Levinson et al.	2002/0183786 A1	12/2002	Girton
6,482,224 B1	11/2002	Michler et al.	2002/0183787 A1	12/2002	Wahr et al.
6,488,706 B1	12/2002	Solymar et al.	2002/0183823 A1	12/2002	Pappu
6,494,846 B1	12/2002	Margolis	2002/0198563 A1	12/2002	Gainor et al.
6,494,888 B1	12/2002	Laufer et al.	2003/0004533 A1	1/2003	Dieck et al.
6,508,828 B1	1/2003	Akerfeldt et al.	2003/0023266 A1	1/2003	Borillo et al.
6,514,515 B1	2/2003	Williams	2003/0028213 A1	2/2003	Thill et al.
6,548,569 B1	4/2003	Williams et al.	2003/0045893 A1	3/2003	Ginn
6,551,303 B1	4/2003	Van Tassel et al.	2003/0050665 A1	3/2003	Ginn
6,551,344 B2	4/2003	Thill	2003/0055455 A1	3/2003	Yang et al.
6,585,719 B2	7/2003	Wang	2003/0057156 A1	3/2003	Peterson et al.
6,585,755 B2	7/2003	Jackson et al.	2003/0059640 A1	3/2003	Marton et al.
6,596,013 B2	7/2003	Yang et al.	2003/0065379 A1	4/2003	Babbas et al.
6,599,448 B1	7/2003	Ehrhard, Jr. et al.	2003/0100920 A1	5/2003	Akin et al.
6,610,764 B1	8/2003	Martin et al.	2003/0120337 A1	6/2003	Van Tassel et al.
6,623,508 B2	9/2003	Shaw et al.	2003/0139819 A1	7/2003	Beer et al.
6,623,518 B2	9/2003	Thompson et al.	2003/0171774 A1	9/2003	Freudenthal et al.
6,626,936 B2	9/2003	Stinson	2003/0191495 A1	10/2003	Ryan et al.
6,629,901 B2	10/2003	Huang	2003/0195530 A1	10/2003	Thill
6,666,861 B1	12/2003	Grabek	2003/0204203 A1	10/2003	Khairkhahan et al.
6,669,722 B2	12/2003	Chen et al.	2004/0044361 A1	3/2004	Frazier et al.
6,689,589 B2	2/2004	Huisman et al.	2004/0073242 A1	4/2004	Chanduszko
6,712,804 B2	3/2004	Roue et al.	2004/0176799 A1	9/2004	Chanduszko et al.
6,712,836 B1	3/2004	Berg et al.	2004/0210301 A1	10/2004	Obermiller
6,726,696 B1	4/2004	Houser et al.	2004/0234567 A1	11/2004	Dawson
6,828,357 B1	12/2004	Martin et al.	2005/0025809 A1	2/2005	Hasirci et al.
6,838,493 B2	1/2005	Williams et al.	2005/0043759 A1	2/2005	Chanduszko
6,867,247 B2	3/2005	Williams et al.	2005/0113868 A1	5/2005	Devellian et al.
6,867,248 B1	3/2005	Martin et al.	2005/0267523 A1	12/2005	Devellian et al.

2005/0273135 A1 12/2005 Chanduszko et al.
 2005/0288786 A1 12/2005 Chanduszko
 2006/0122647 A1 6/2006 Callaghan et al.
 2006/0265004 A1 11/2006 Callaghan et al.
 2007/0010851 A1 1/2007 Chanduszko et al.
 2007/0167981 A1 7/2007 Opolski

FOREIGN PATENT DOCUMENTS

EP 0362113 4/1990
 EP 0474887 A1 3/1992
 EP 0 839 549 5/1998
 EP 0839549 A1 5/1998
 EP 0 861 632 9/1998
 EP 1013227 A2 6/2000
 EP 1046375 A1 10/2000
 EP 1222897 A2 7/2002
 WO WO-96/25179 A1 8/1996
 WO WO-96/31157 A1 10/1996
 WO WO-98/07375 A1 2/1998
 WO WO 98/08462 3/1998
 WO WO 98/16174 4/1998
 WO WO-98/29026 7/1998
 WO WO-98/51812 11/1998
 WO WO-99/05977 A1 2/1999
 WO WO-98/18864 4/1999
 WO WO-99/18862 A1 4/1999
 WO WO-99/18864 4/1999
 WO WO-99/18870 A1 4/1999
 WO WO-99/18871 A1 4/1999
 WO WO-99/30640 A1 6/1999
 WO WO-00/27292 A1 5/2000
 WO WO-00/44428 A2 8/2000
 WO WO-01/08600 2/2001
 WO WO-01/19256 3/2001
 WO WO-01/21247 A1 3/2001
 WO WO-01/28432 4/2001
 WO WO-01/30268 A1 5/2001
 WO WO-01/49185 A1 7/2001
 WO WO-01/78596 A1 10/2001
 WO WO-01/93783 12/2001
 WO WO-02/17809 A1 3/2002
 WO WO-02/24106 A3 3/2002
 WO WO-03/024337 3/2003
 WO WO-03/053493 A1 7/2003
 WO WO-03/53493 A2 7/2003
 WO WO-03/059152 7/2003
 WO WO-03/063732 A 8/2003
 WO WO-03/077733 A2 9/2003
 WO WO-03/082076 10/2003
 WO WO-03/103476 12/2003
 WO WO-2004/032993 4/2004
 WO WO-2004/037333 5/2004
 WO WO-2004/043266 5/2004
 WO WO-2004/043508 5/2004
 WO WO-2004/052213 6/2004
 WO WO-2005/006990 1/2005
 WO WO-2005/018728 3/2005
 WO WO-2005/027752 3/2005
 WO WO-2005/074813 8/2005
 WO WO-2005/092203 10/2005
 WO WO-2005/110240 11/2005
 WO WO-2005/112779 12/2005
 WO WO-2006/036837 4/2006
 WO WO-2006/102213 9/2006

OTHER PUBLICATIONS

Athanasion, T., "Coronary Artery Bypass with the Use of a Magnetic Distal Anastomotic Device: Surgical Technique and Preliminary Experience," *The Heart Surgery Forum* #2004-1024, 2004, 4 pgs.

Bachthaler, M. et al., "Corrosion of Tungsten Coils After Peripheral Vascular Embolization Therapy: Influence on Outcome and Tungsten Load", *Catherization and Cardiovascular Interventions*, vol. 62, pp. 380-384, 2004.

Barroso, L.A. et al., "RPM: A Rapid Prototyping Engine for Multi-processor Systems", *IEEE Computer*, Feb. 1995, pp. 26-34.

Berg SLT/MST Connector System, Berg Electronics, Du Pont Bulletin, 1260, Oct. 1983.

Boxer, A. "Where Buses Cannot Go", *IEEE Spectrum*, Feb. 1995, pp. 41-45.

Connector System for Transmission-Line Cables, Wilding, Eleventh Annual Connector Symposium Proceedings, pp. 308-316, Oct. 1978.

Definition of "adverse", 1996, Microsoft Bookshelf Basics, The American Heritage Dictionary of the English Language, 3.sup.rd edition, Houghton Mifflin Co., INSO Corp.

European Examination Report, European Application No. 03779297.5, mailed Mar. 15, 2007 (6 pgs.).

European Examination Report, European Application No. 04781644.2, mailed Aug. 23, 2007 (3 pgs).

European Search Report, European Application No. 03729663.9, mailed Feb. 20, 2008 (3 pgs).

Falk, V., "Facilitated Endoscopic Beating Heart Coronary Artery Bypass Grafting Using a Magentic Coupling Device," *Journal of Thoracic and Cardiovascular Surgery*, vol. 126,(5), pp. 1575-1579.

Filsoufi, F., et al., "Automated Distal Coronary Bypass with a Novel Magnetic Coupler (MVP system)," *J. Thoracic and Cardiovascular Surgery*, vol. 127(1), pp. 185-192.

Huang, X., et al. Passive Mode-Locking in 1.3 μm Two-Section InAs Quantum Dot Lasers, *Applied Physics Letters*, 2001, vol. 78(19) pp. 2825-2828.

Huang, Y., et al "Logic Gates and Computation from Assembled Nanowire Building Blocks," *Science*, Nov. 9, 2001, vol. 294, pp. 1313-1316.

Imholt, T. J., "Nanotubes in Microwave Fields: Light Emission, Intense Heat, Outgassing, and Reconstructin," Downloaded from Web, 2004, pp. 1-2.

International Search Report for International Patent Application No. PCT/AU03/00759, filed Jun. 19, 2003.

International Search Report, International Application No. PCT/US02/40850 mailed Jun. 19, 2003 (4 pgs).

International Search Report, International Application No. PCT/US03/01050, mailed Jul. 8, 2003 (1 pg).

International Search Report, International Application No. PCT/US03/09051, mailed Sep. 29, 2003 (2 pgs).

International Search Report, International Application No. PCT/US03/17390 mailed Oct. 6, 2003 (4 pgs).

International Search Report, International Application No. PCT/US03/17715, mailed Mar. 24, 2004 (2 pgs).

International Search Report, International Application No. PCT/US03/32133, mailed Apr. 22, 2004 (1 pg).

International Search Report, International Application No. PCT/US03/34003 mailed Oct. 3, 2004 (4 pgs).

International Search Report, International Application No. PCT/US03/35479, mailed Apr. 14, 2004 (2 pgs).

International Search Report, International Application No. PCT/US03/35998 mailed Jun. 16, 2004 (5 pgs).

International Search Report, International Application No. PCT/US03/39253, mailed Apr. 19, 2004 (4 pgs).

International Search Report, International Application No. PCT/US04/022643, mailed Mar. 31, 2005 (2 pgs).

International Search Report, International Application No. PCT/US04/026998, mailed Apr. 22, 2005 (5 pgs).

International Search Report, International Application No. PCT/US04/029978, mailed Jan. 26, 2005 (3 pgs).

International Search Report, International Application No. PCT/US05/006703, mailed Jul. 25, 2005 (3 pgs).

International Search Report, International Application No. PCT/US05/013705 mailed Aug. 4, 2005 (4 pgs).

International Search Report, International Application No. PCT/US05/015382, mailed Oct. 6, 2005 (4 pgs).

International Search Report, International Application No. PCT/US05/34276, mailed 9 Oct. 2007.

- International Search Report, International Application No. PCT/US06/009978, mailed Jul. 13, 2006 (2 pgs).
- International Search Report, International Application No. PCT/US07/065546, mailed 29 Oct. 2007 (4 pgs).
- International Search Report, International Application No. PCT/US2007/065541, mailed Aug. 7, 2007 (4 pgs).
- International Search Report, International Application No. PCT/US97/14822, mailed Feb. 20, 1998 (2 pgs).
- International Search Report, International Application No. PCT/US97/17927, mailed Feb. 10, 1998 (1 pg).
- Islam, M. F. et al., "High Weight Fraction Surfactant Solubilization of Single-Wall Carbon Nanotubes in Water," *Nano Letters*, Jan. 16, 2003, vol. 3, No. 2, pp. 269-273.
- Isotalo, T. et al., "Biocompatibility Testing of a New Bioabsorbable X-Ray Positive SR-PLA 96/4 Urethral Stent", *The Journal of Urology*, vol. 163, pp. 1764-1767, Nov. 1999.
- Javey, A., et al., "Carbon Nanotube Transistor Arrays for Multistage Complementary Logic and Ring Oscillators," *Nano Letters*, 2002, vol. 2, No. 9, pp. 929-932.
- Kimura, A., et al., "Effects of Neutron Irradiation on the Transformation Behavior in Ti-Ni Alloys," Abstract, Proceedings of the Int'l Conf. On Martensitic Transformations, 1992, pp. 935-940.
- Klima, U., "Magnetic Vascular Port in Minimally Invasive Direct Coronary Artery Bypass Grafting," *Circulation*, 2004, 11-55 -11-60.
- Meier, MD, Bernhard et al., "Contemporary Management of Patent Foramen Ovale," American Heart Association, Inc., *Circulation*, 2003, vol. 107, pp. 5-9.
- Nat'l Aeronautics and Space Administration, "55-Nitinol—The Alloy with a Memory: Its Physical Metallurgy, Properties, and Applications," NASA Report, pp. 24-25.
- Ogawa et al., *Fiber Diffraction Methods*, 47, pp. 353-362 (1980).
- Parviainen, M. et al., "A New Biodegradable Stent for the Pancreaticojejunal Anastomosis After Pancreaticoduodenal Resection: In Vitro Examination and Pilot Experiences in Humans", *Pancreas*, vol. 21, No. 1, pp. 14-21, 2000.
- Ramanathan, G., et al., "Experimental and Computational Methods for Shape Memory Alloys," 15th ASCE Engineering Mechanics Conference, Jun. 2-5, 2002.
- Ruddy, a.C. et al., "Rheological, Mechanical and Thermal Behaviour of Radipaque Filled Polymers", *Polymer Processing Research Centre, School of Chemical Engineering, Queen's University of Belfast*, 5 pgs.
- Ruiz, et al., "The Puncture Technique: A New Method for Transcatheter Closure of Patent Foramen Ovale," *Catheterization and Cardiovascular Interventions*, 2001, vol. 53, pp. 369-372.
- Shabalovskaya, S., "Surface, Corrosion and Biocompatibility Aspects of Nitinol as an Implant Material," *Bio-Medical Materials and Engineering*, 2002, vol. 12, pp. 69-109.
- Simpson et al., *Microbiology*, vol. 141, pp. 1451-1460 (1995).
- SMST-2000, "Proceedings of the International Conference on Shape Memory and Superelastic Technologies," 30 Apr. To May 4, 2000, Asilomar Conference Center.
- Stein, H., "Telemanipulator-gestützte Applikation eines magnetischen Gefäß-Kopplers am schlagenden Herzen mit dem da Vinci™ -Surgical-System," *Biomedizinische Technik*, 2003, vol. 48(9), pp. 230-234.
- Stockel, "Nitinol Medical Devices and Implants," SMST-2000 Conference Proceedings, 2001, pgs. 531-541.
- Uchil, J., "Shape Memory Alloys—Characterization Techniques," *Pramana—Journal of Physics*, 2002, vol. 58(5)(6), pp. 1131-1139.
- Vaajanen, A. et al., "Expansion and Fixation Properties of a New Braided Biodegradable Urethral Stent: An Experimental Study in the Rabbit", *The Journal of Urology*, vol. 169, pp. 1771-1774, Mar. 2003.
- Virag et al., "Effects of poly (ADP-ribose) polymerase Inhibition on inflammatory cell migration in a murine model of asthma." *Med. Sci. Monit*, 2004, vol. 10, pp. BR77-83.

* cited by examiner

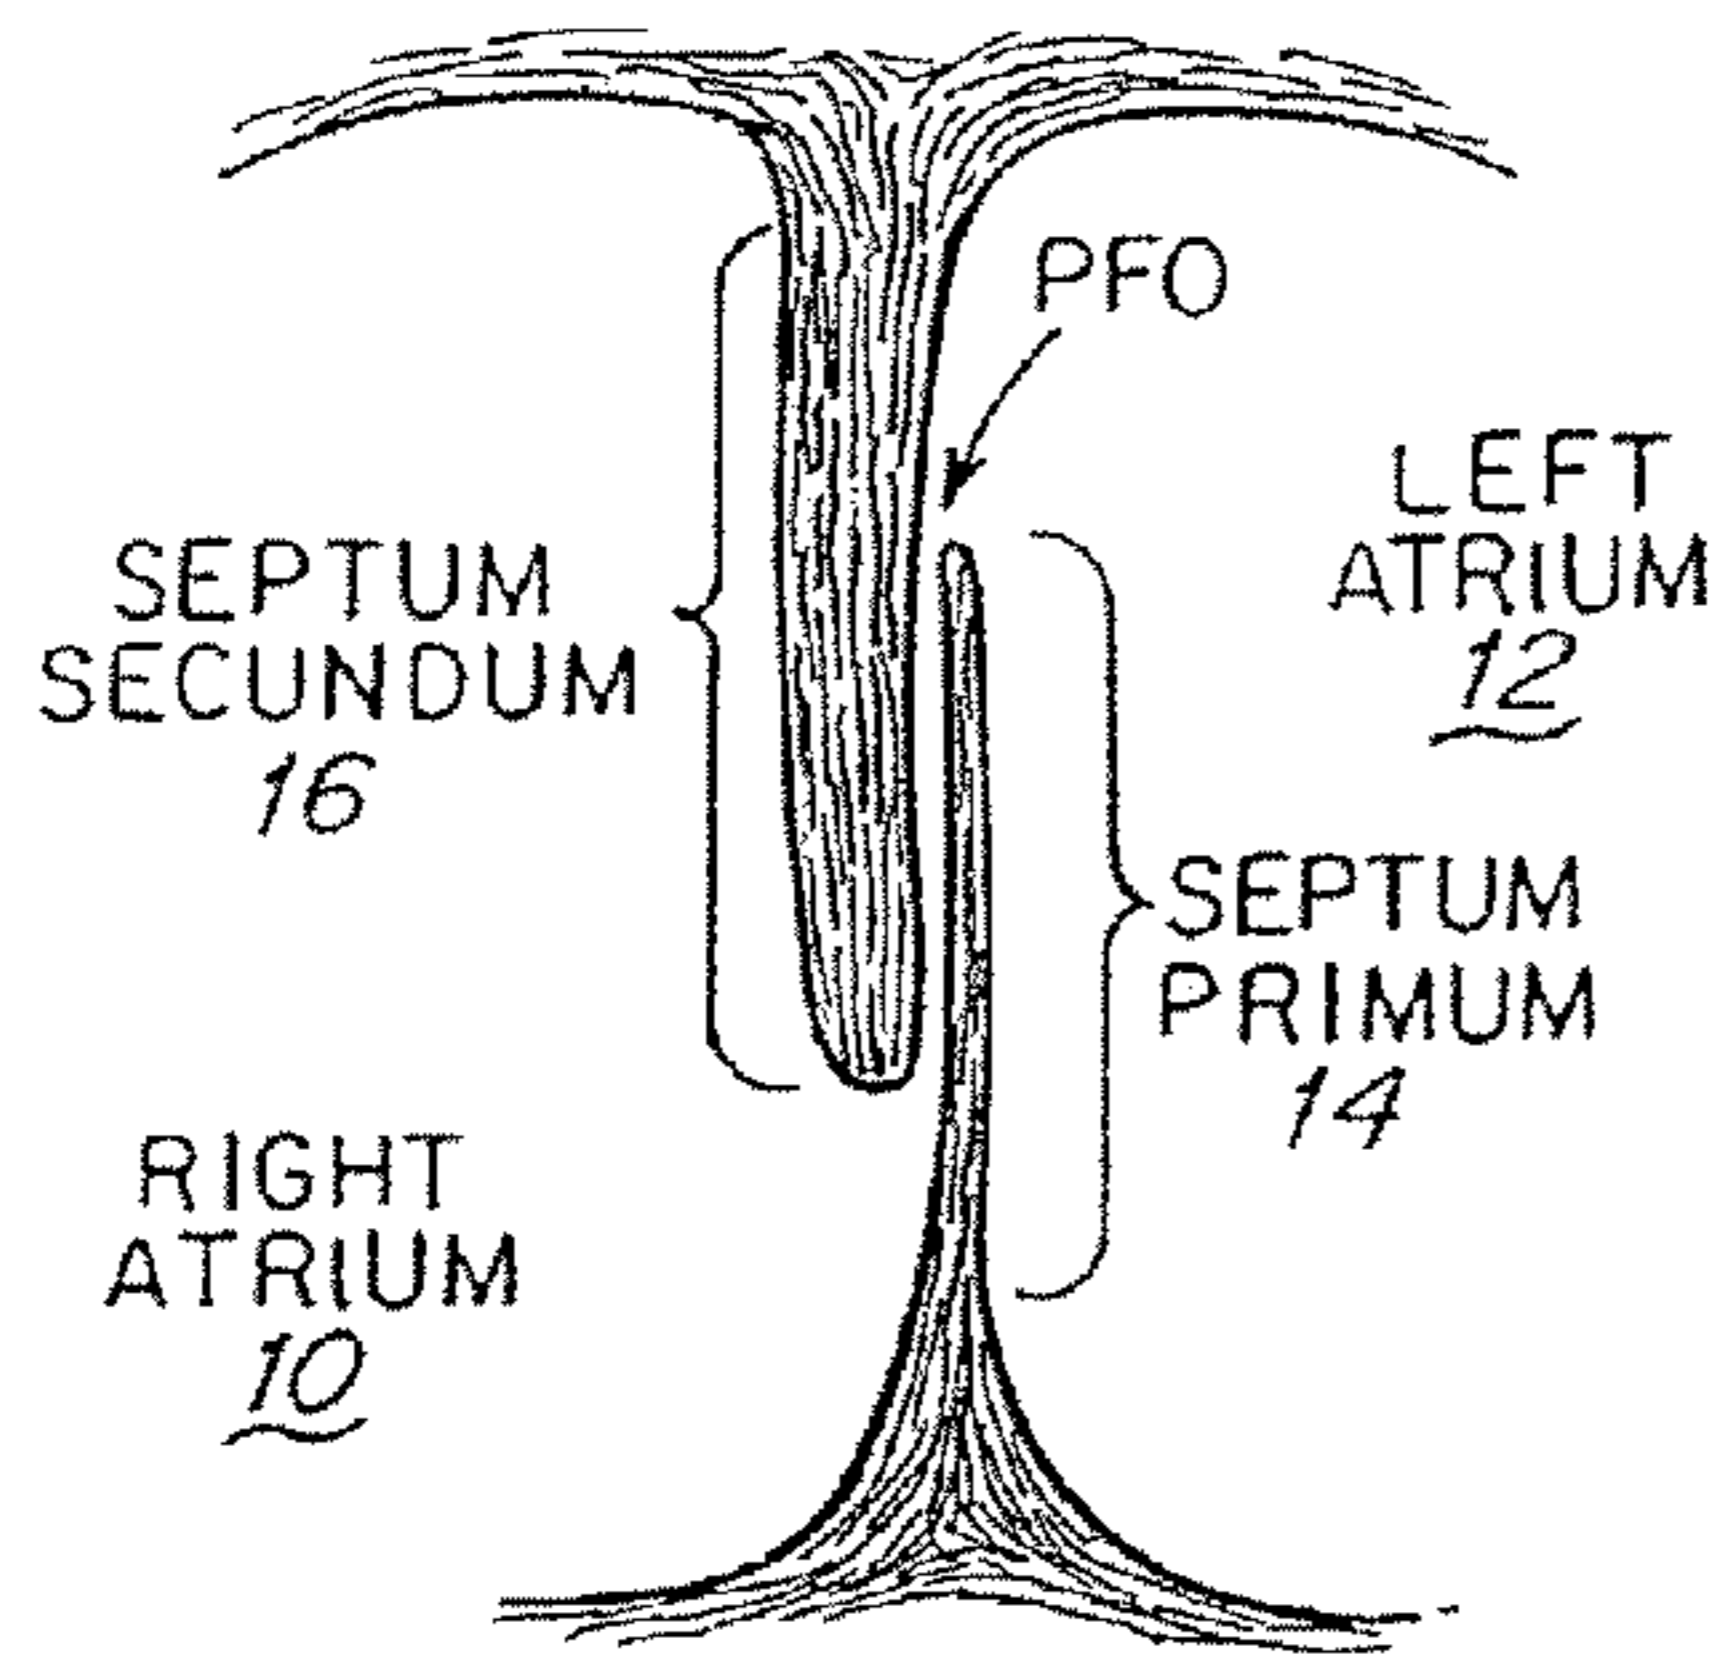


Fig. 1

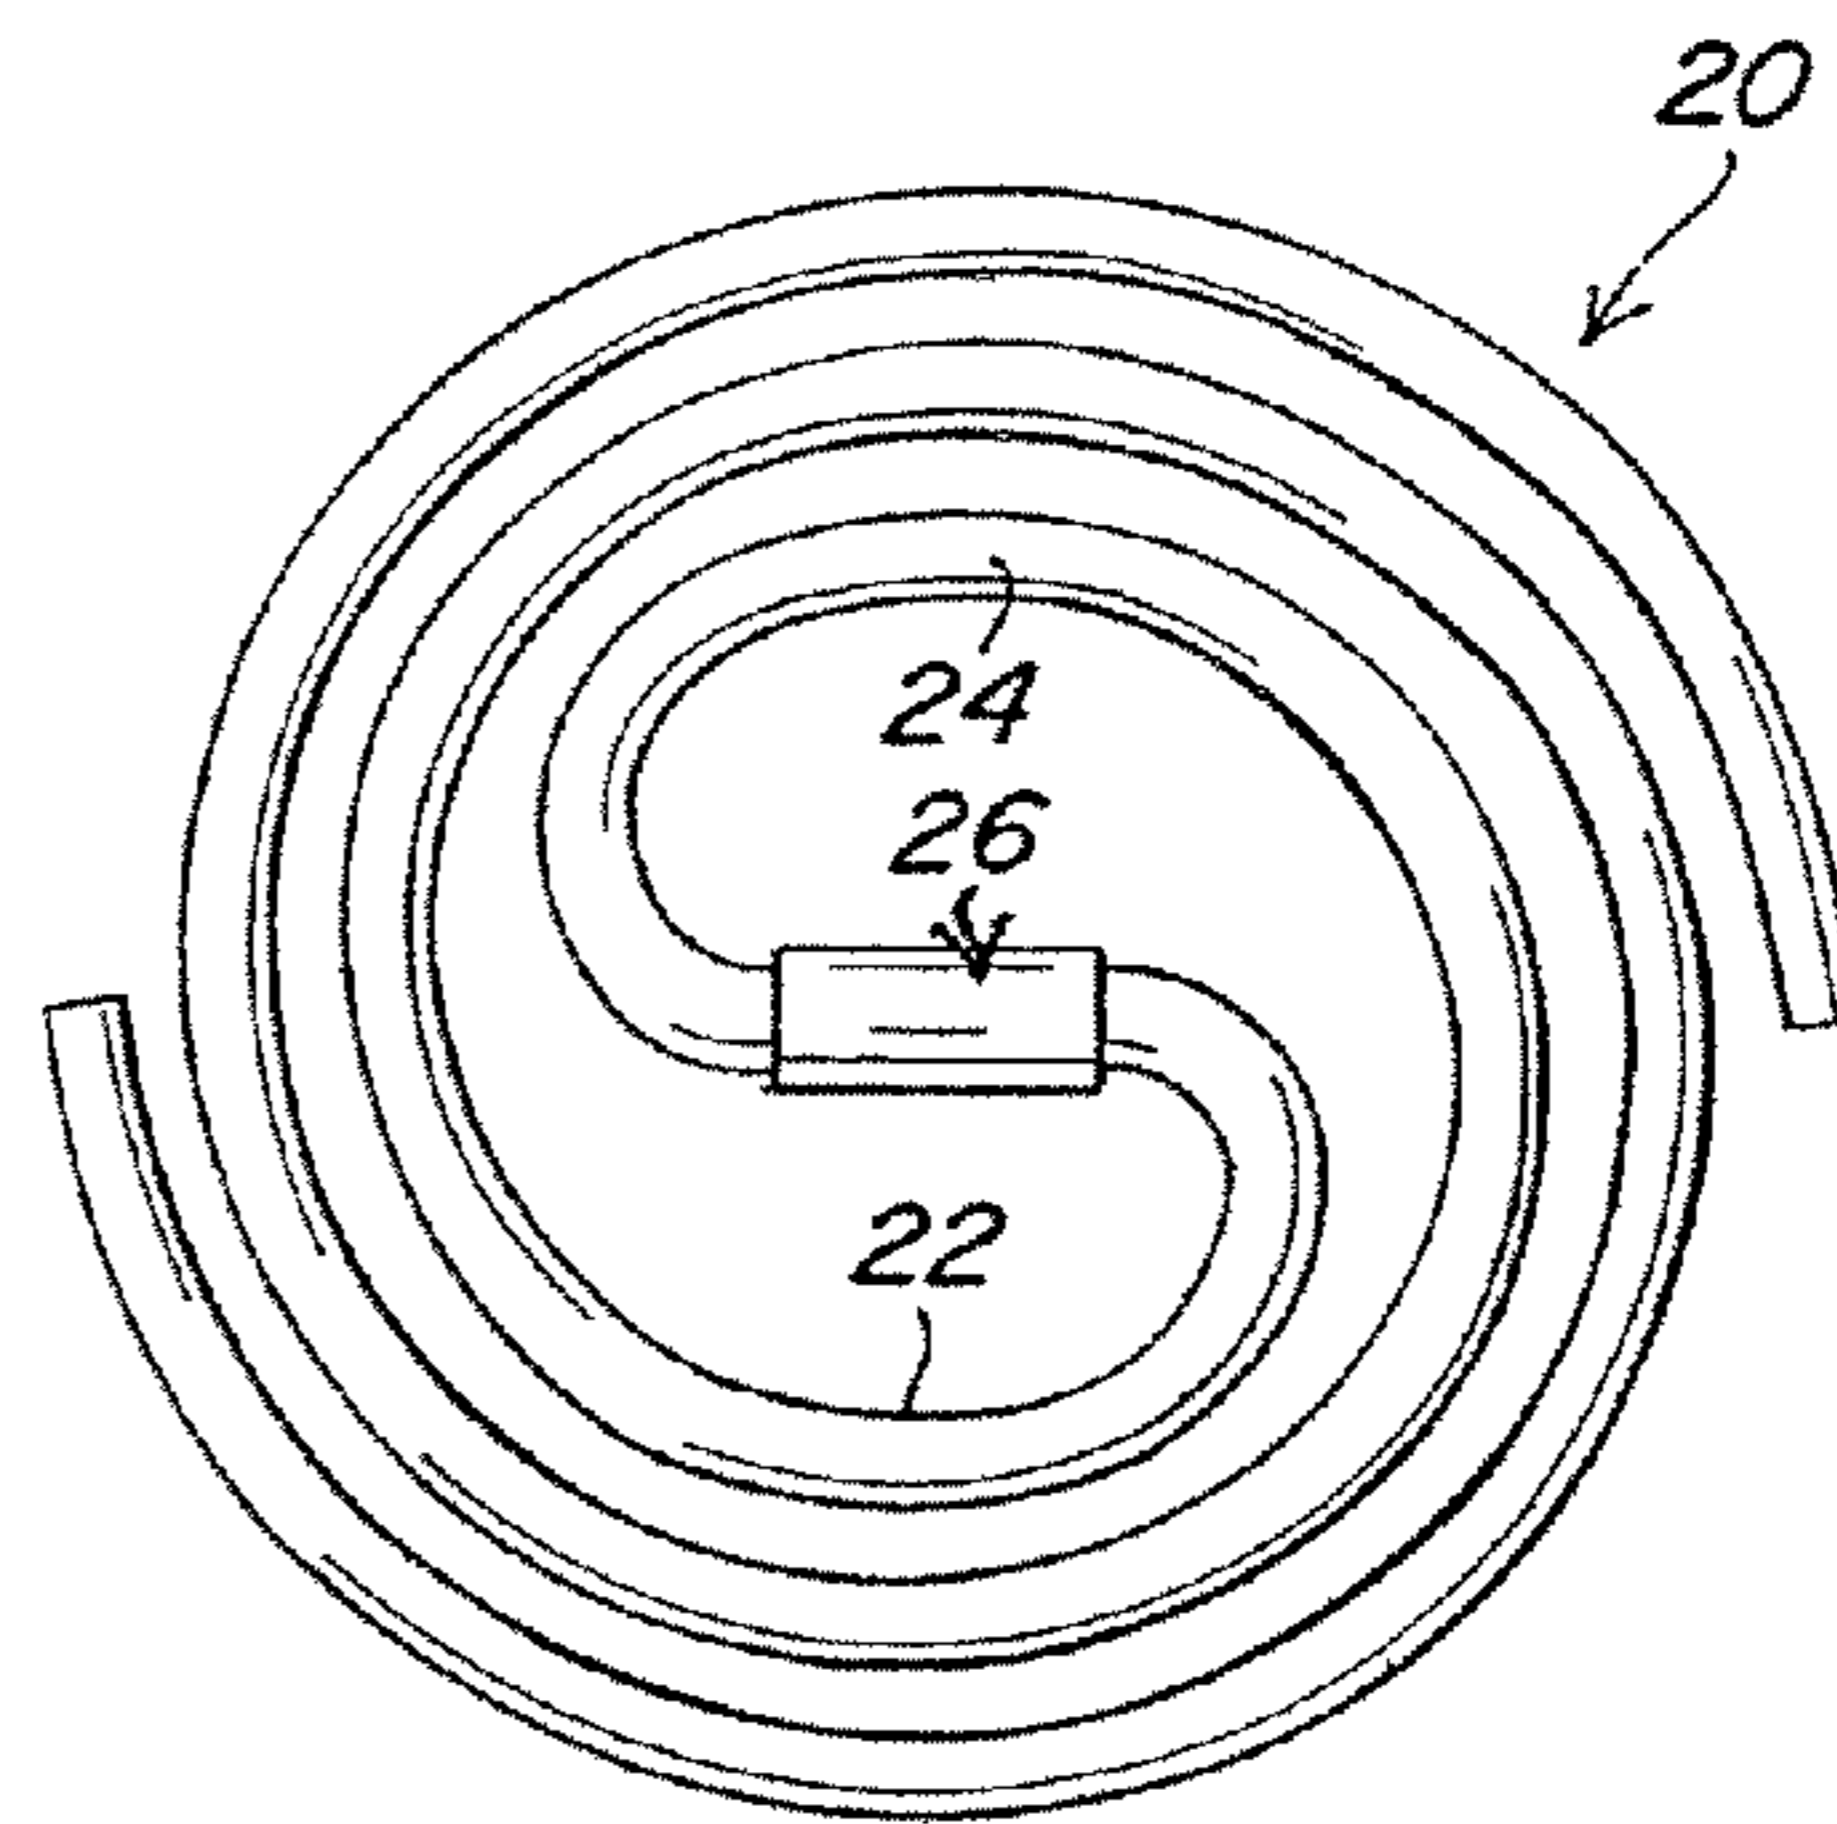


Fig. 2A

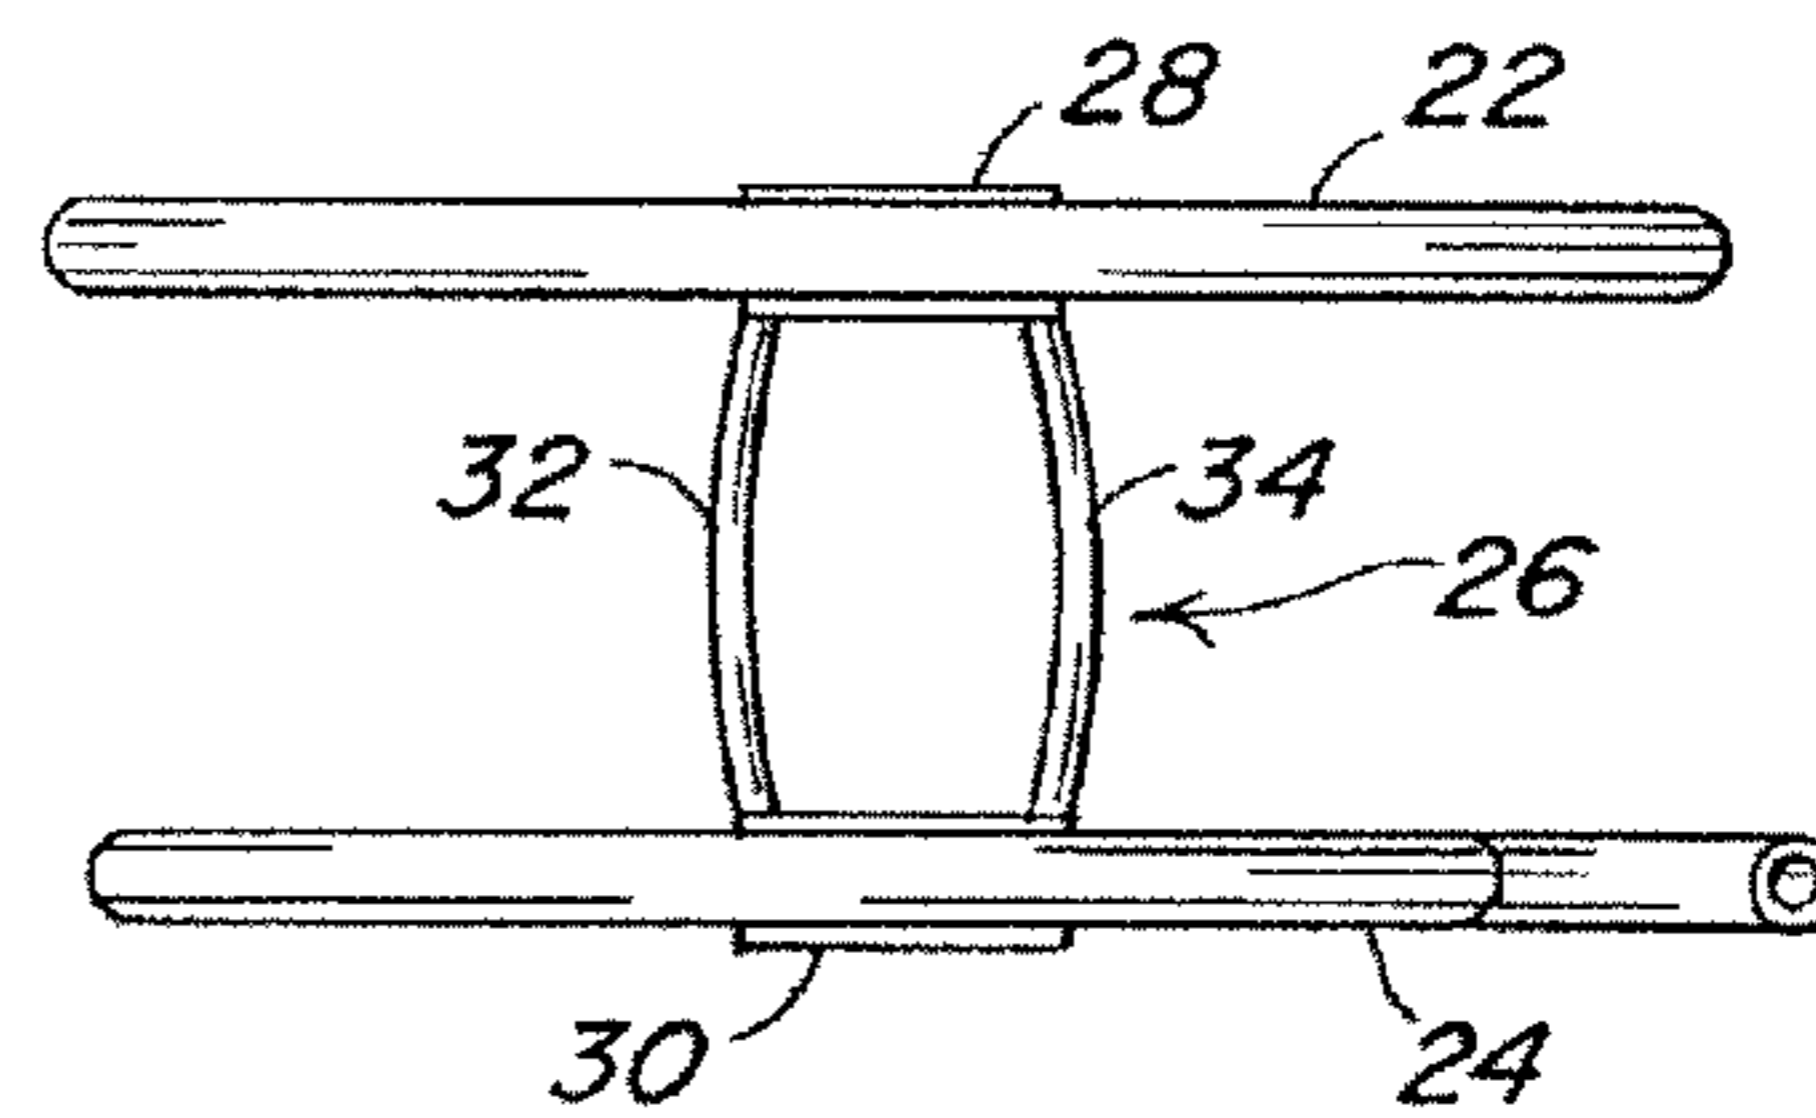


Fig. 2B

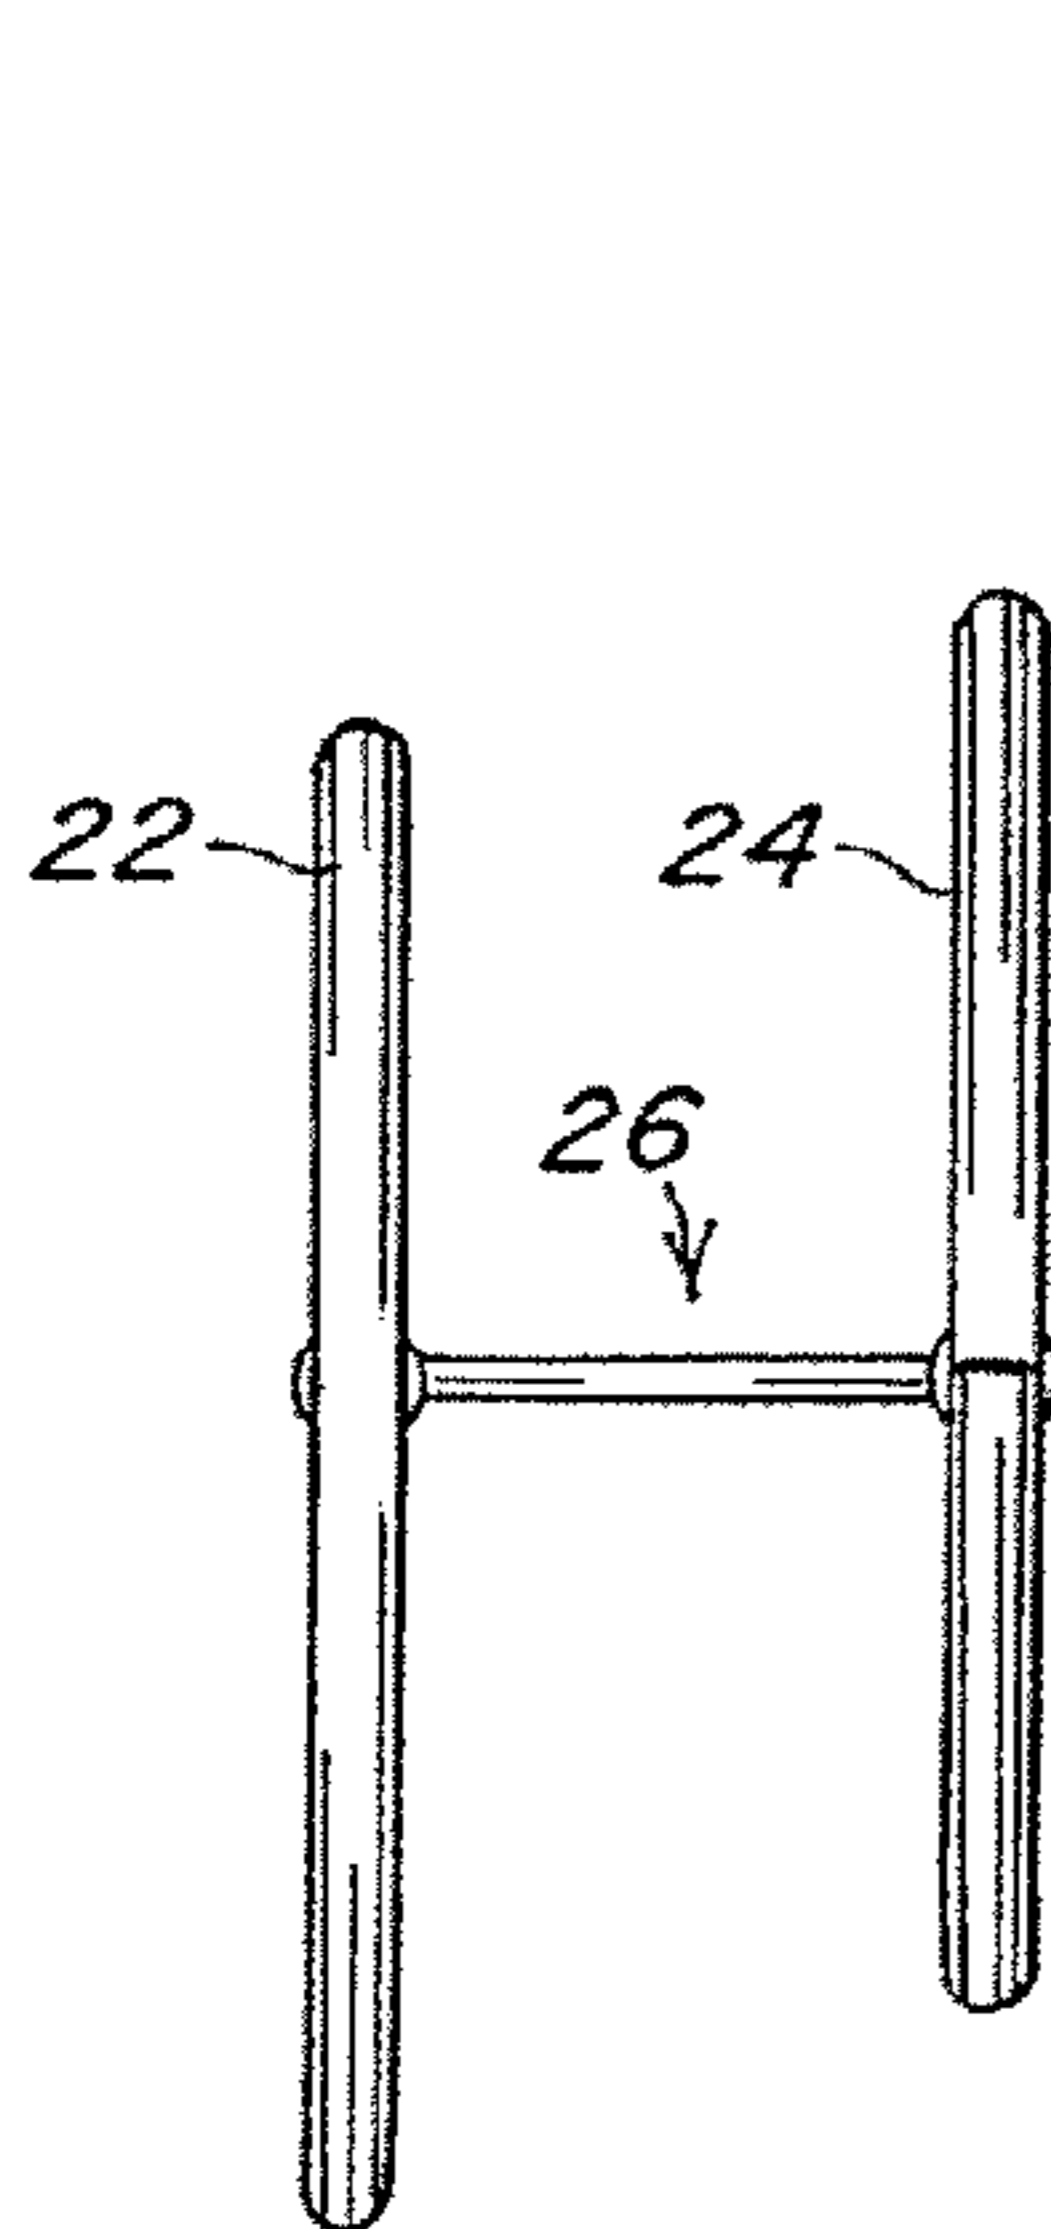


Fig. 3A

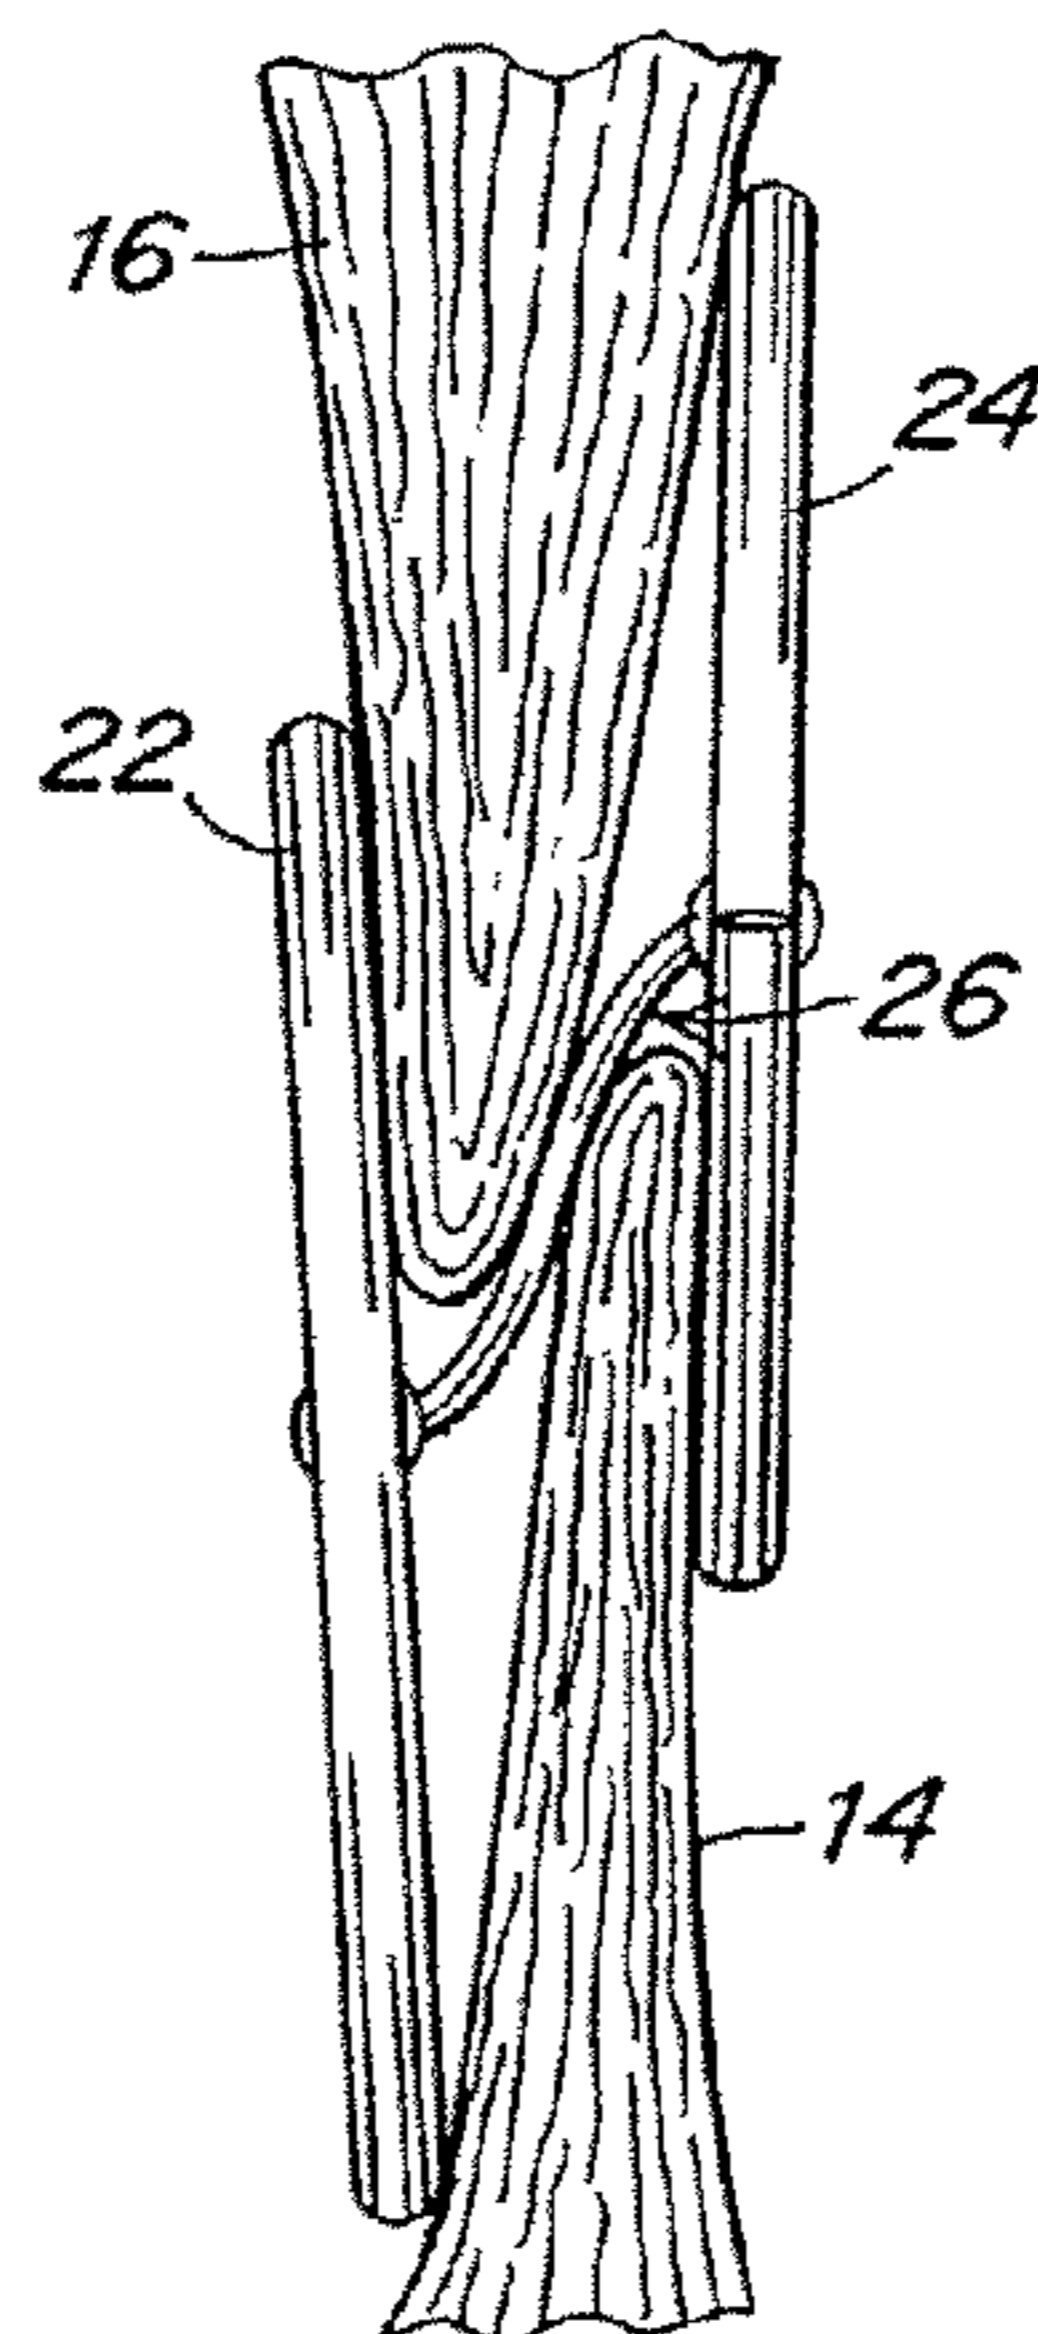


Fig. 3B

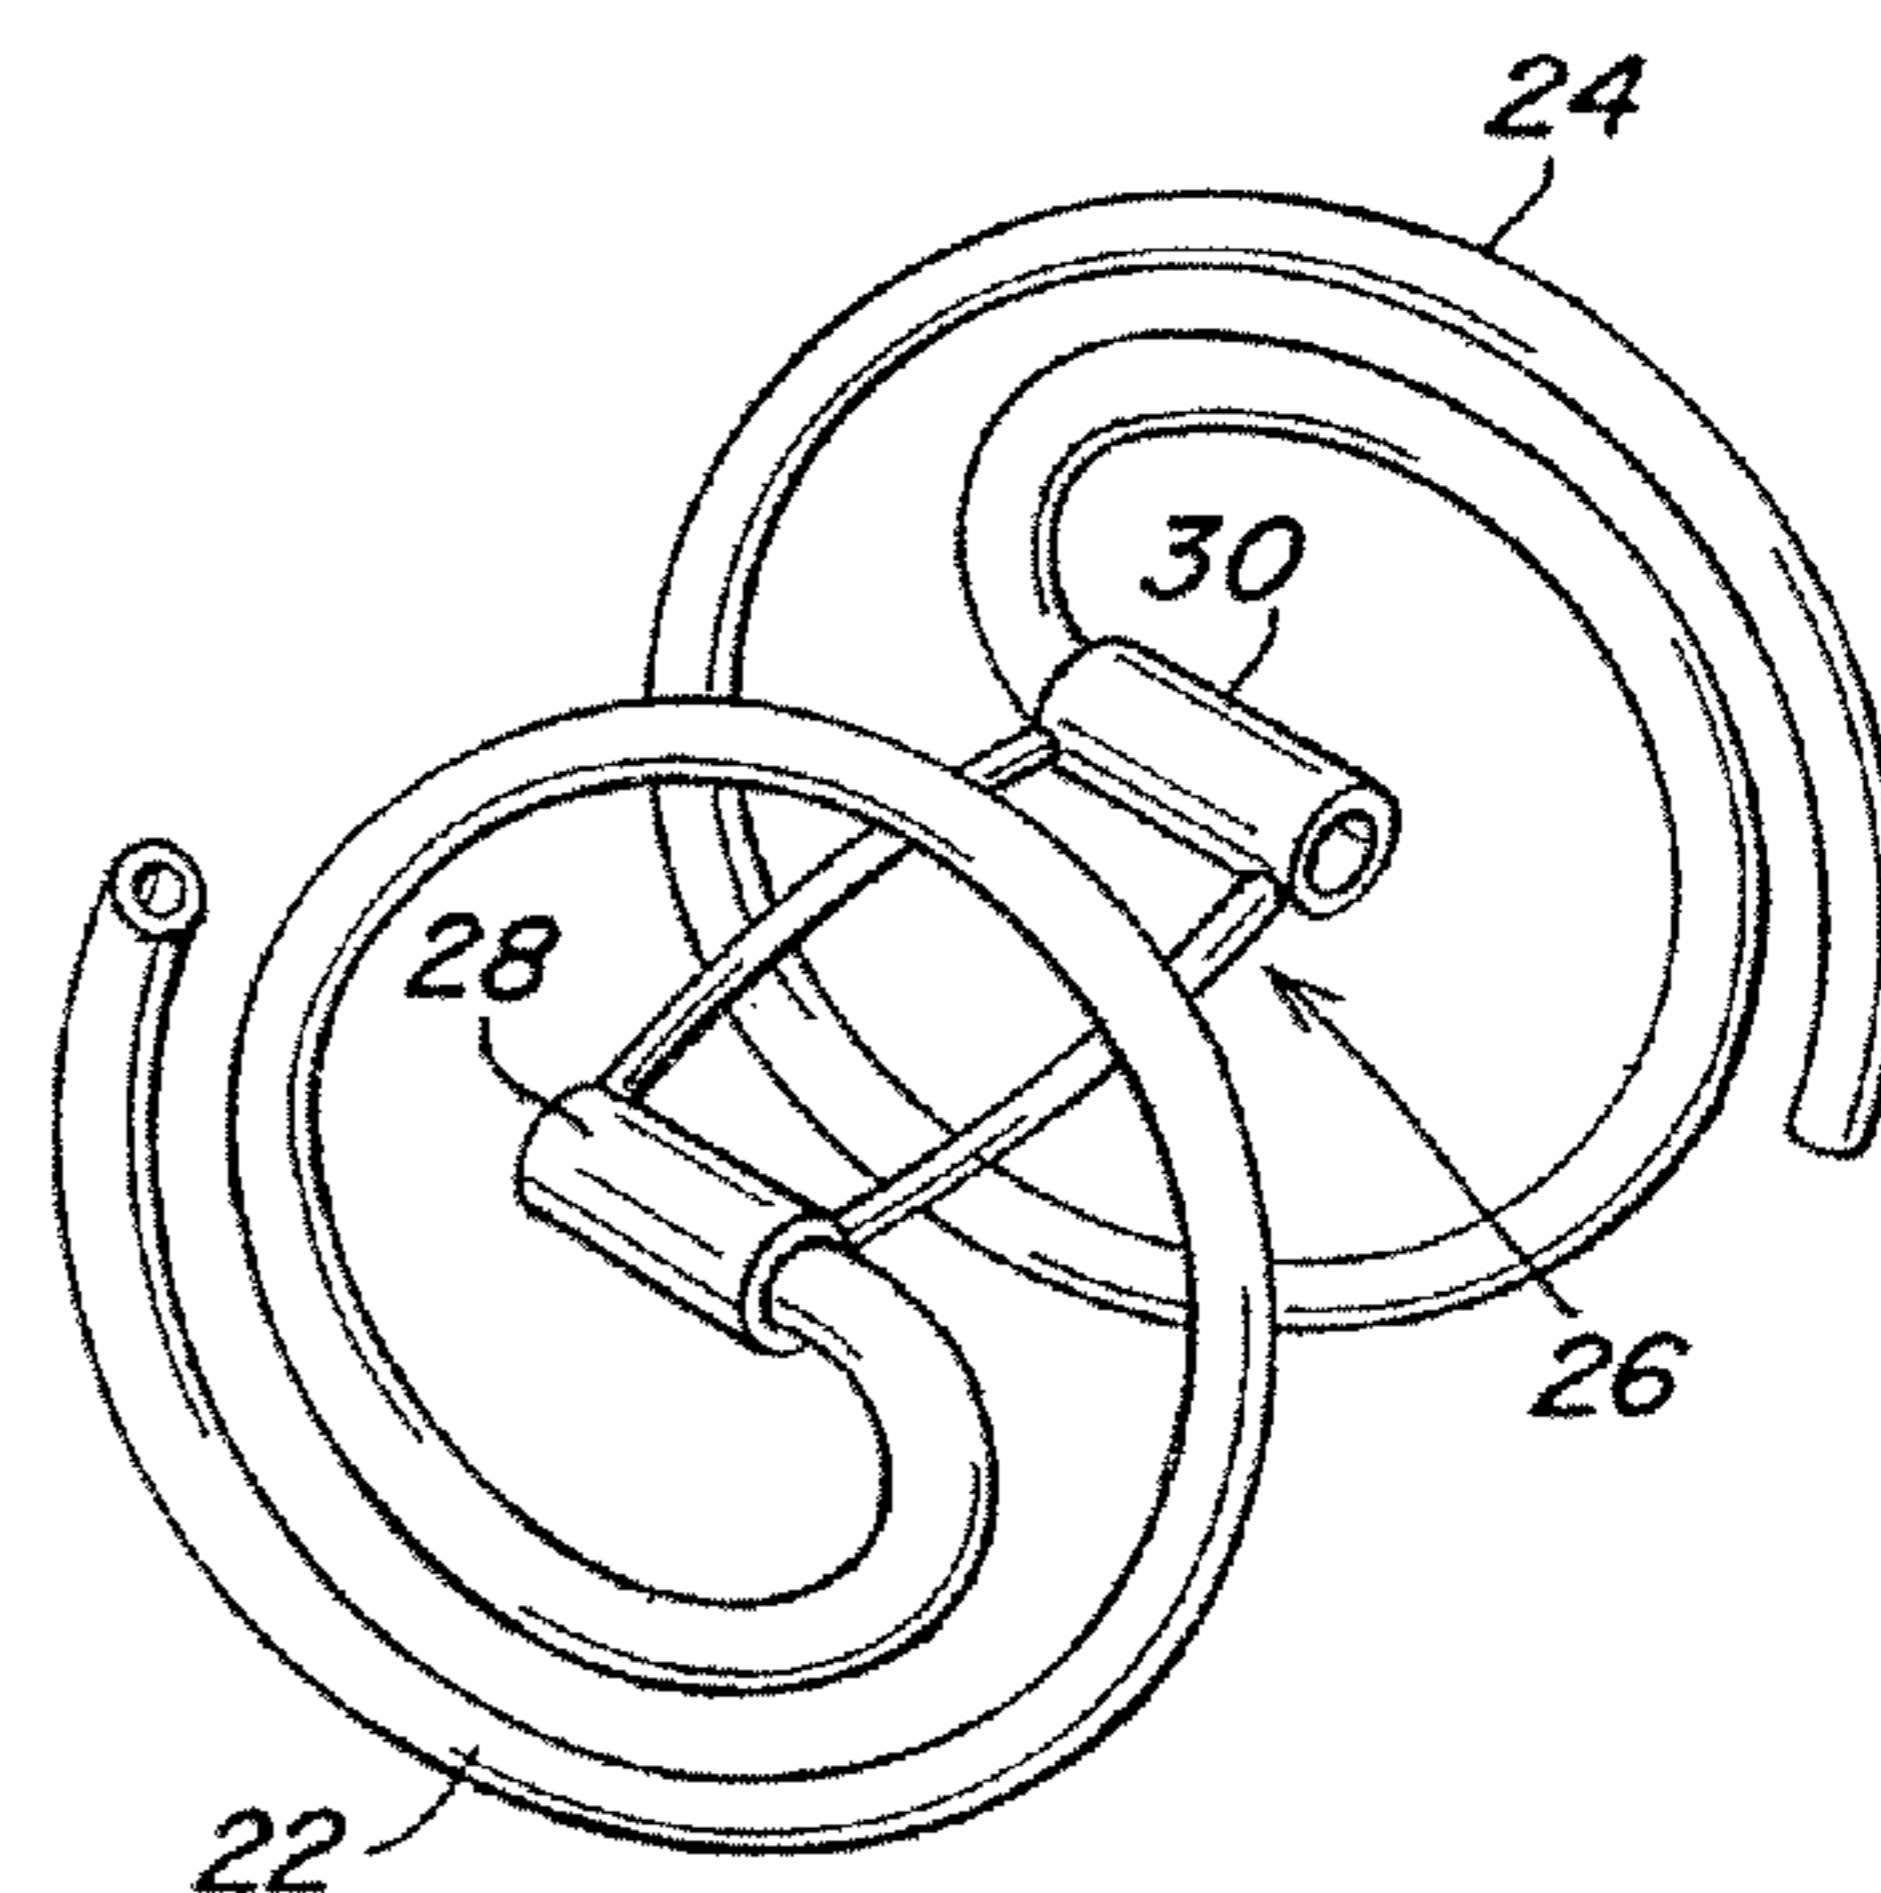


Fig. 4

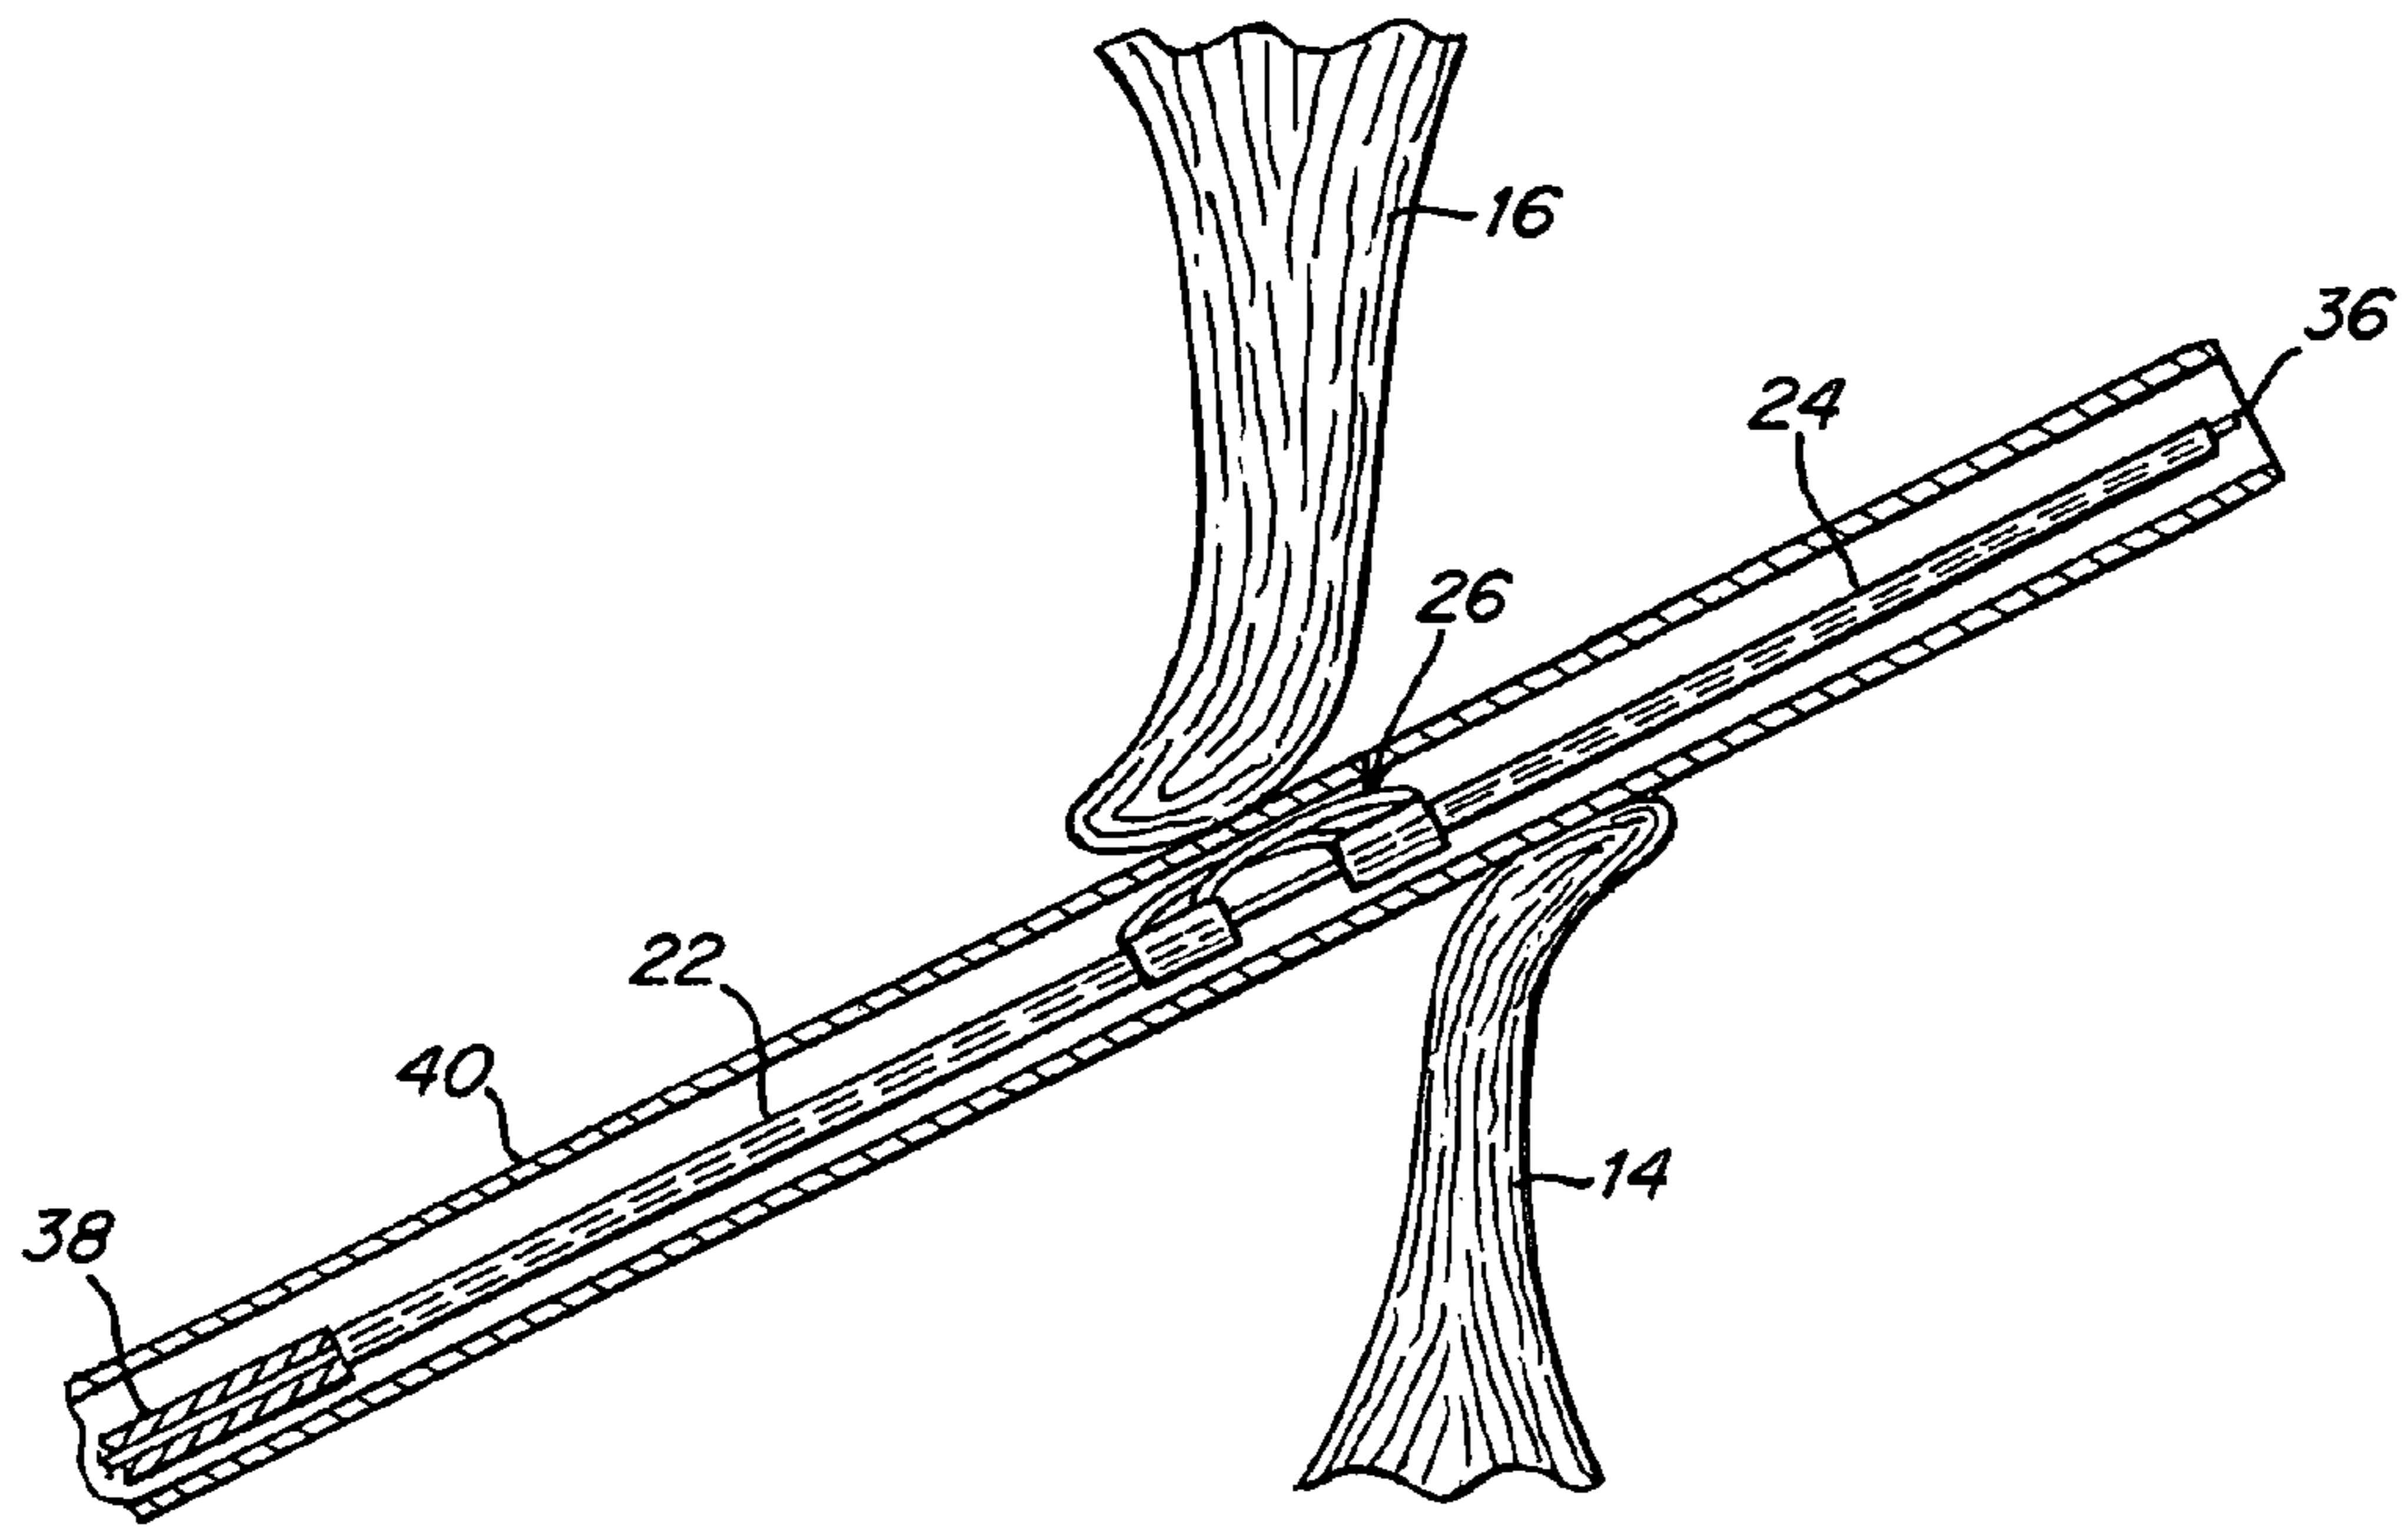


Fig. 5

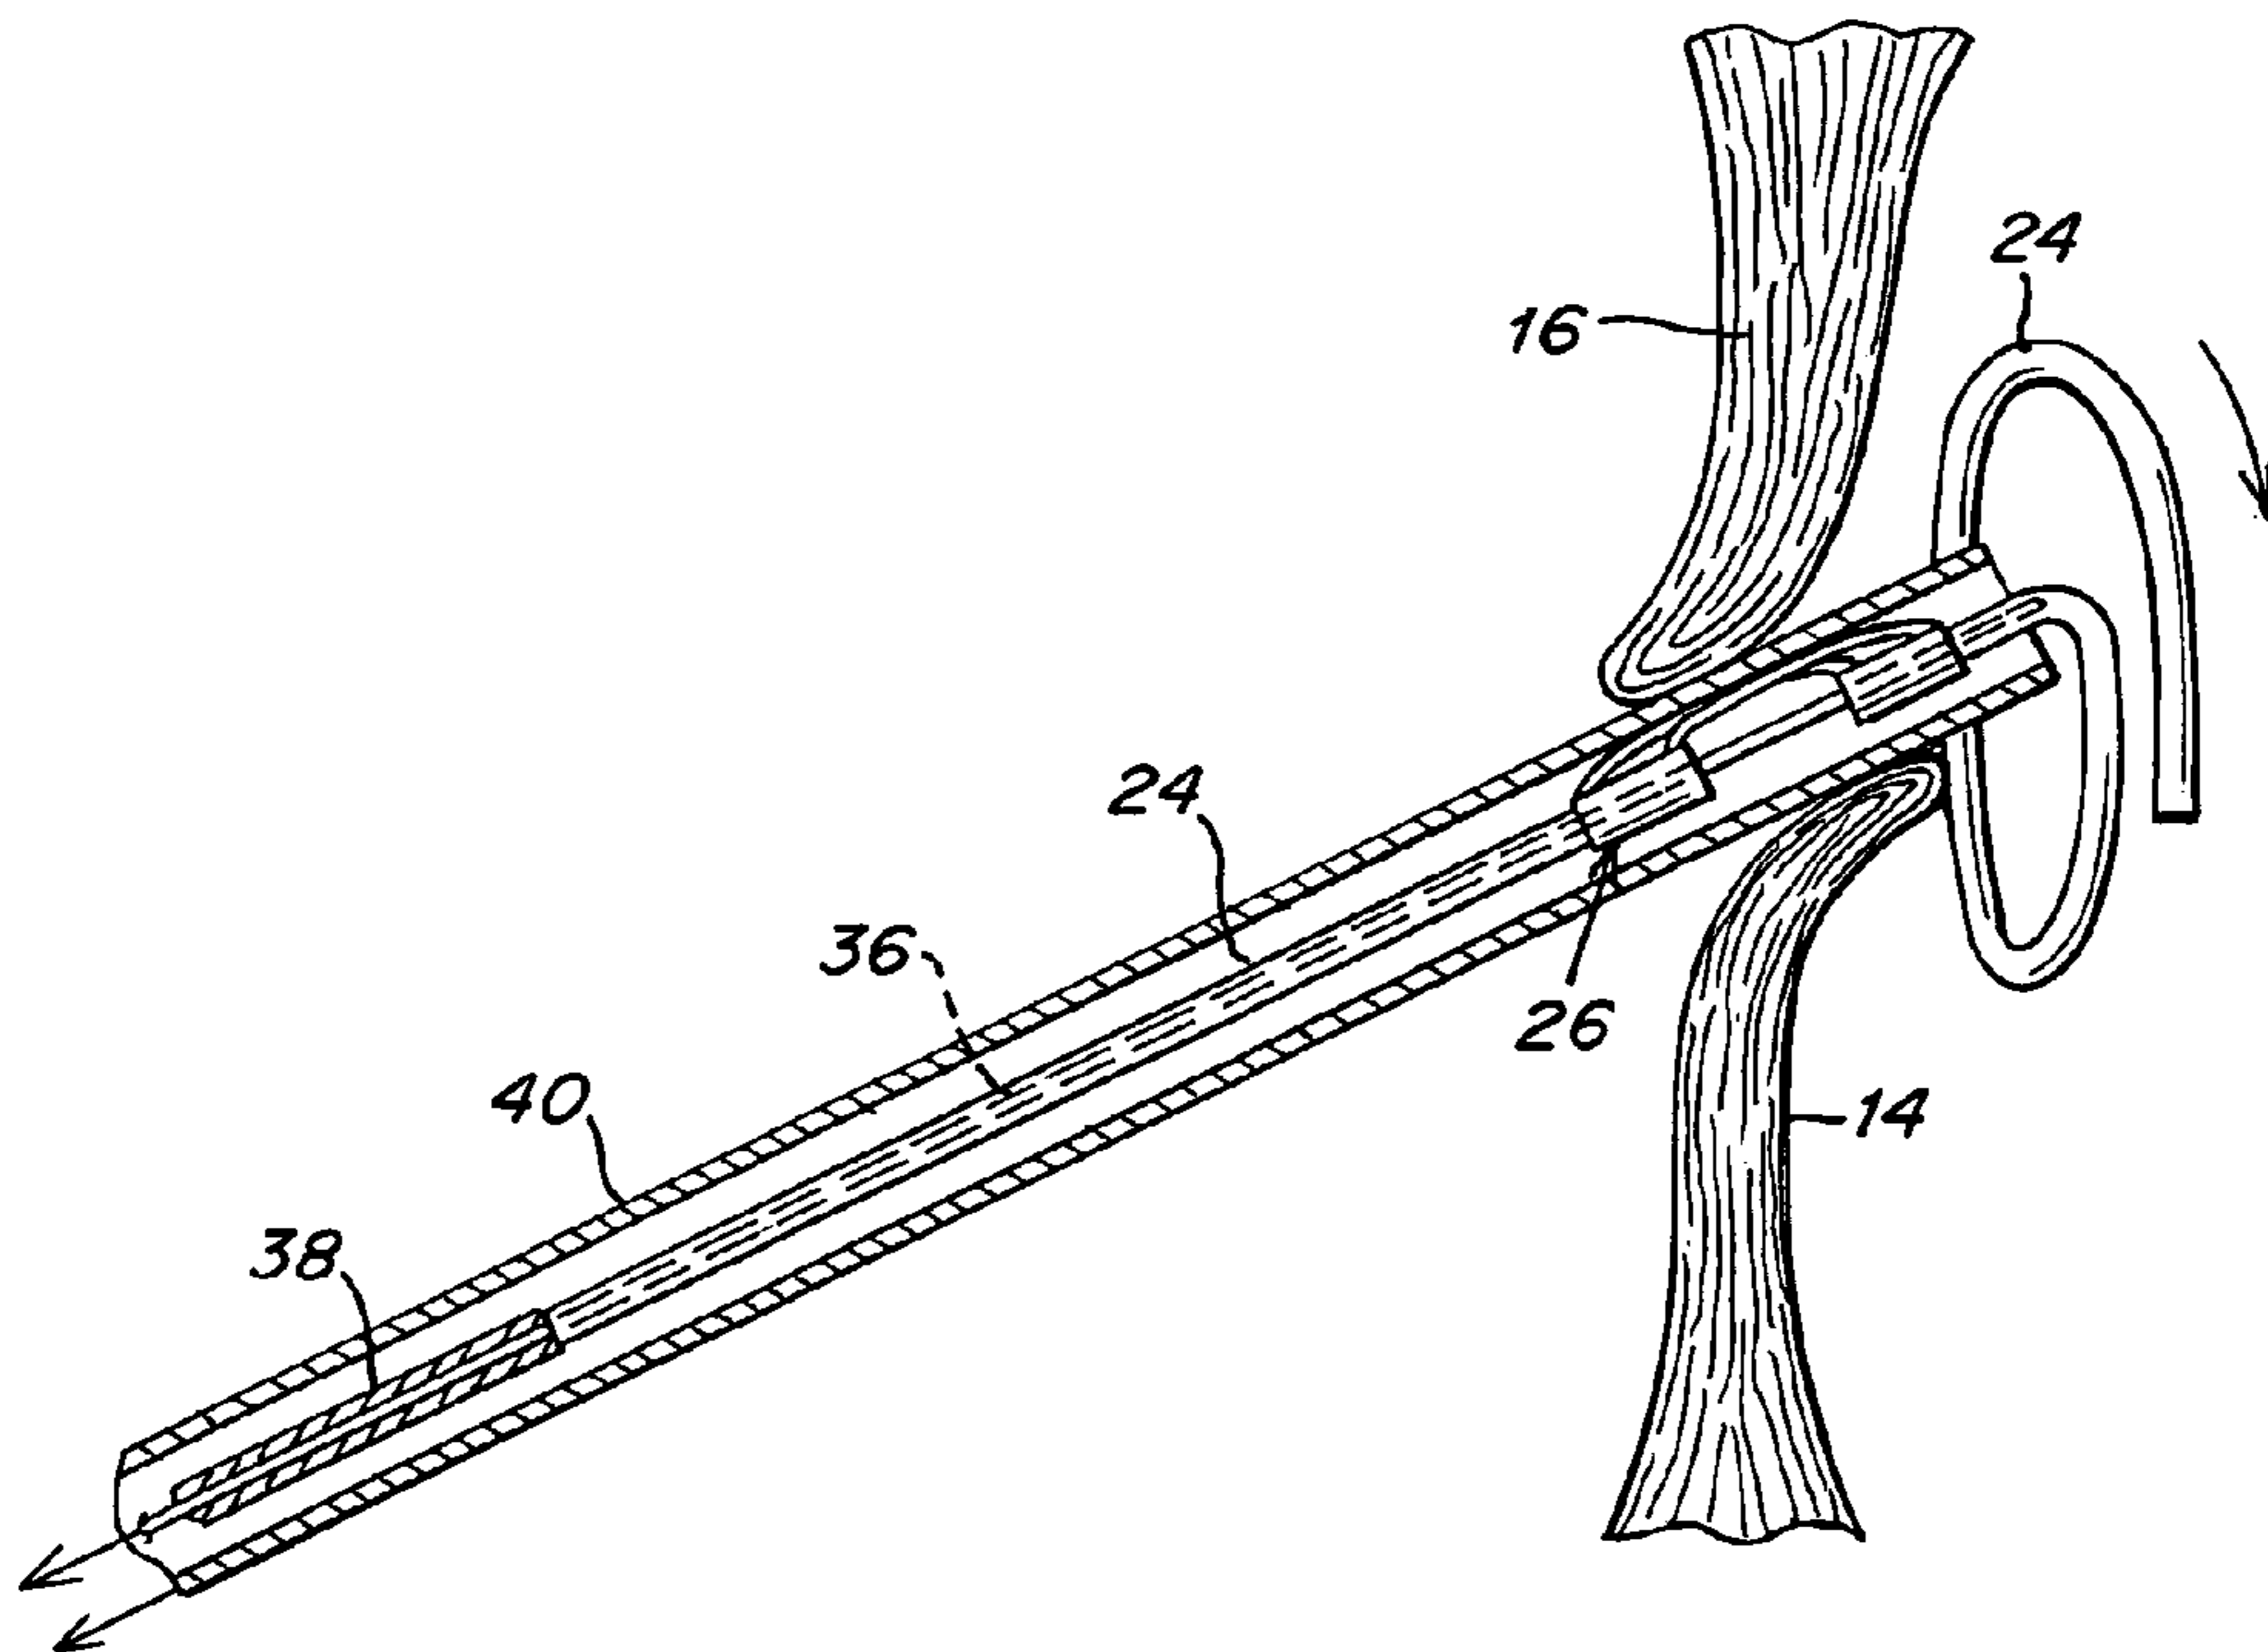


Fig. 6

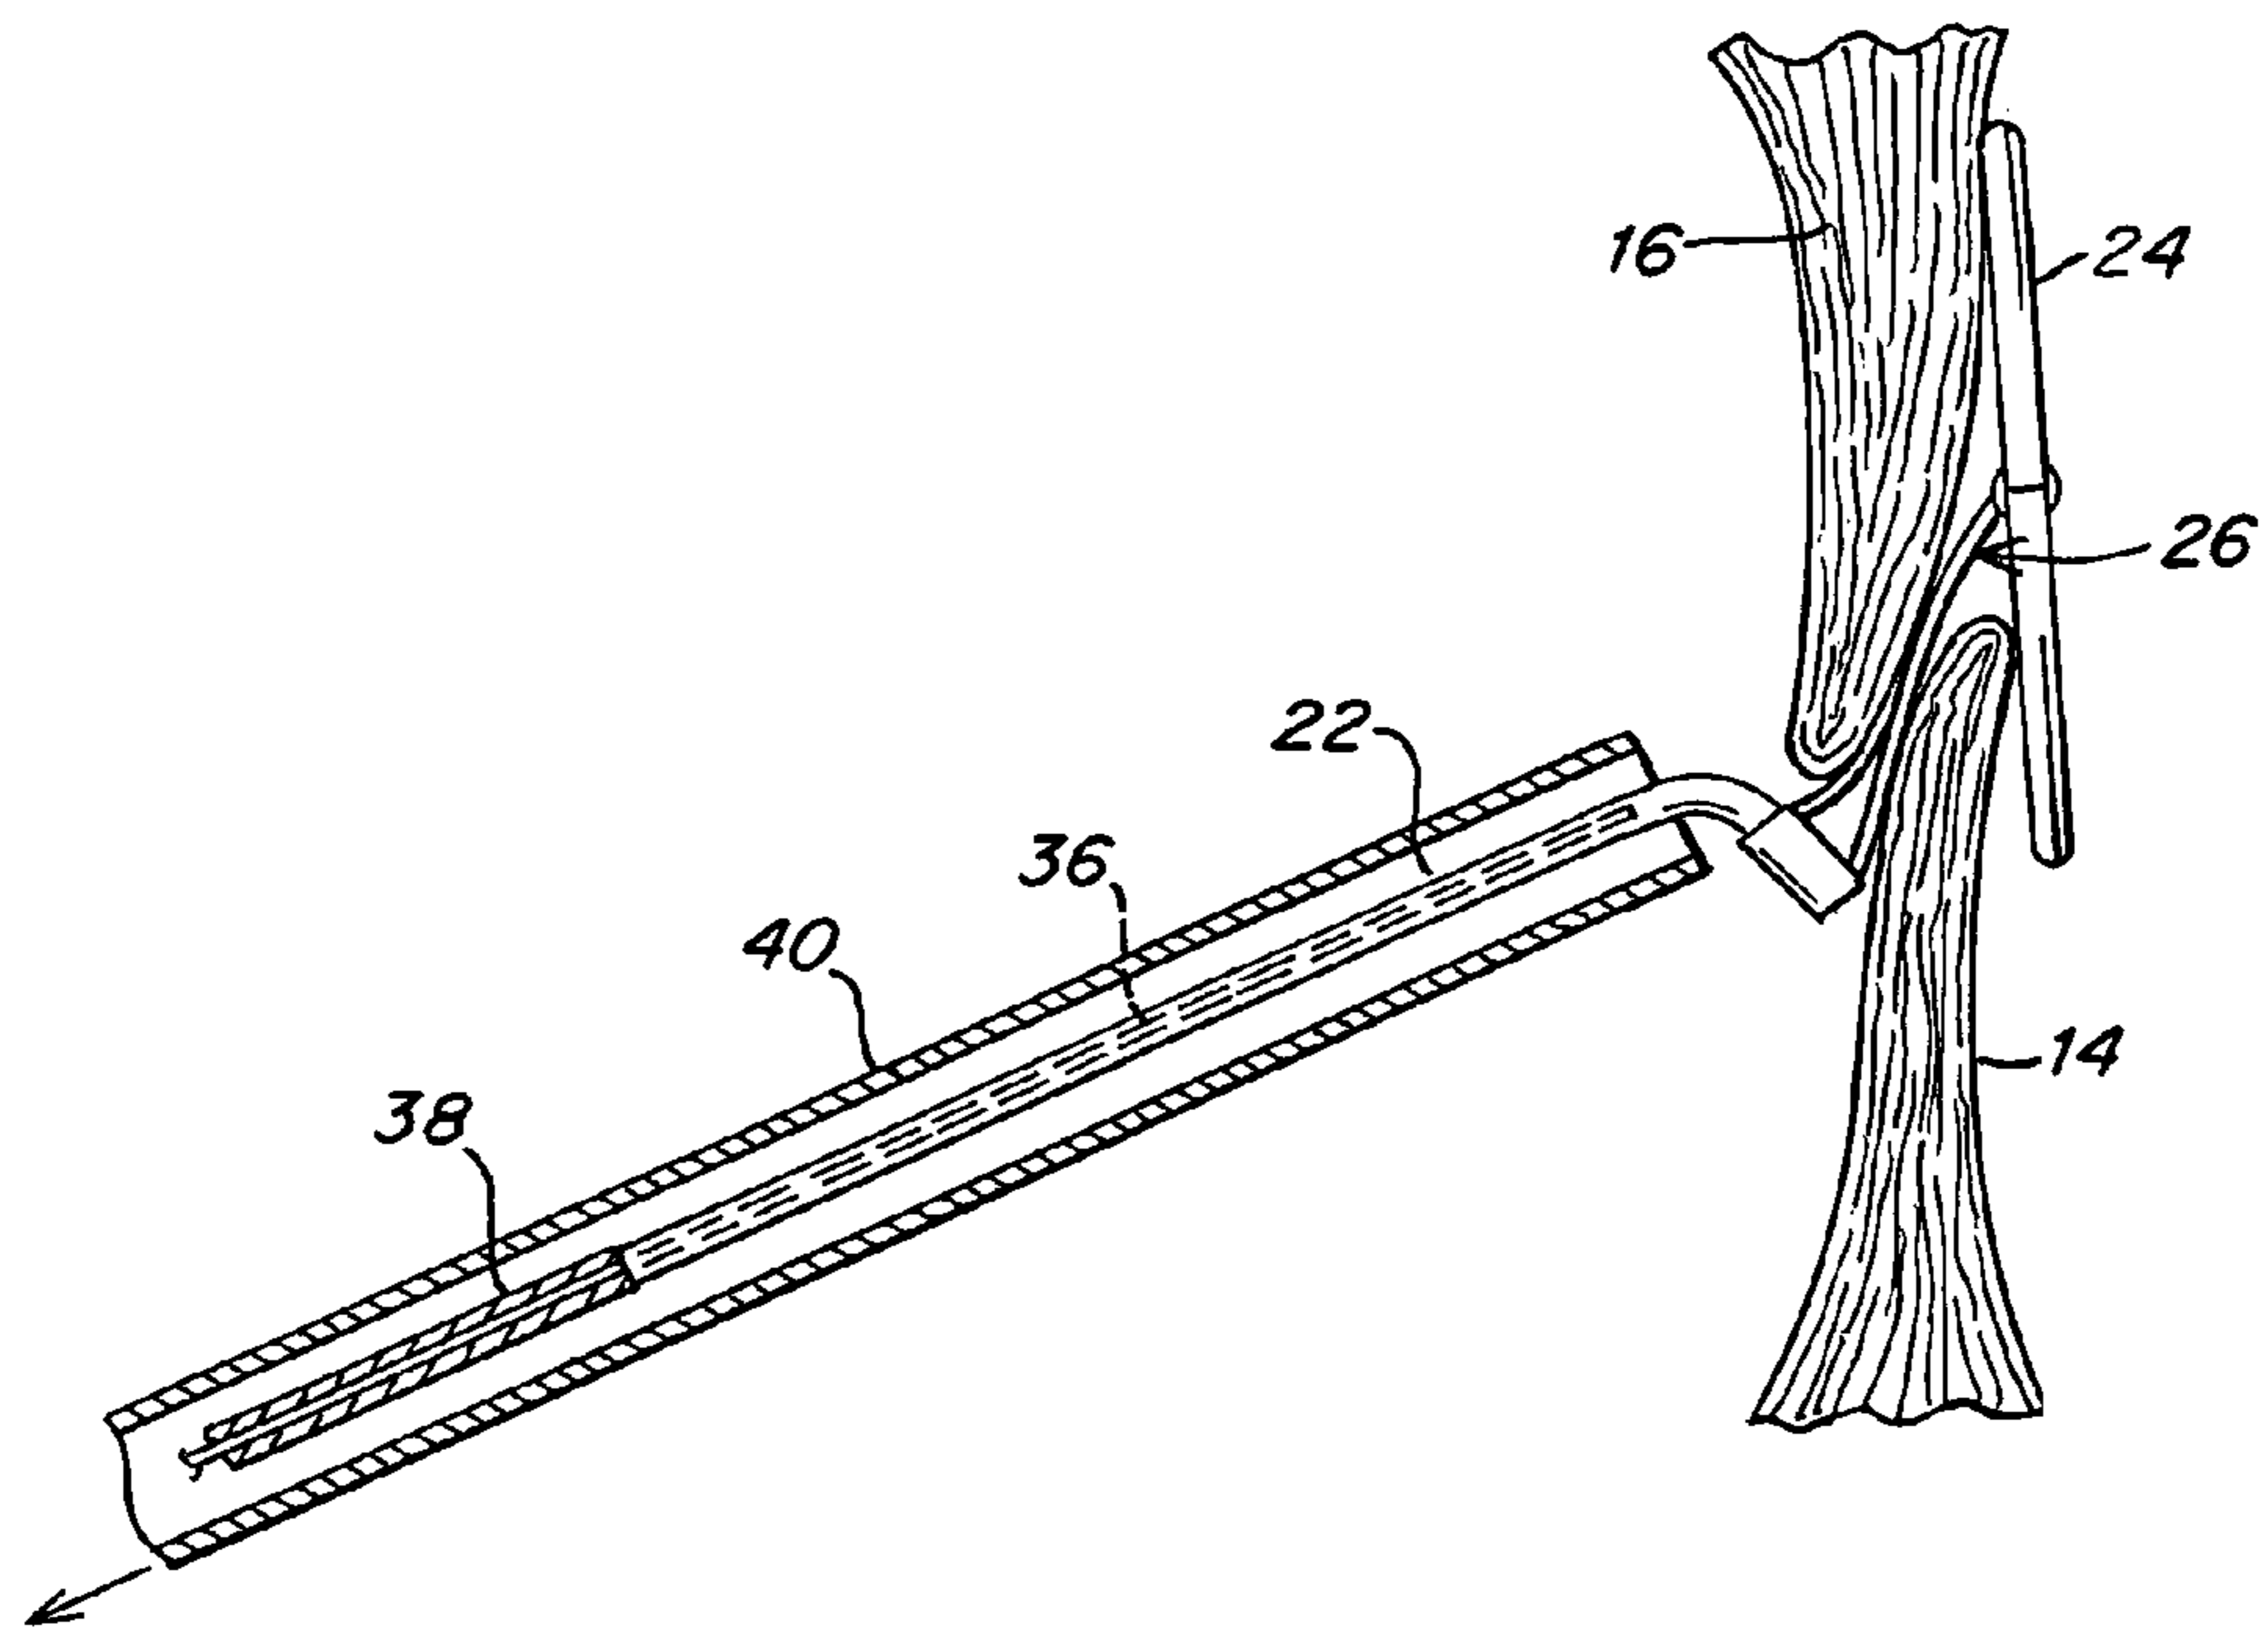


Fig. 7

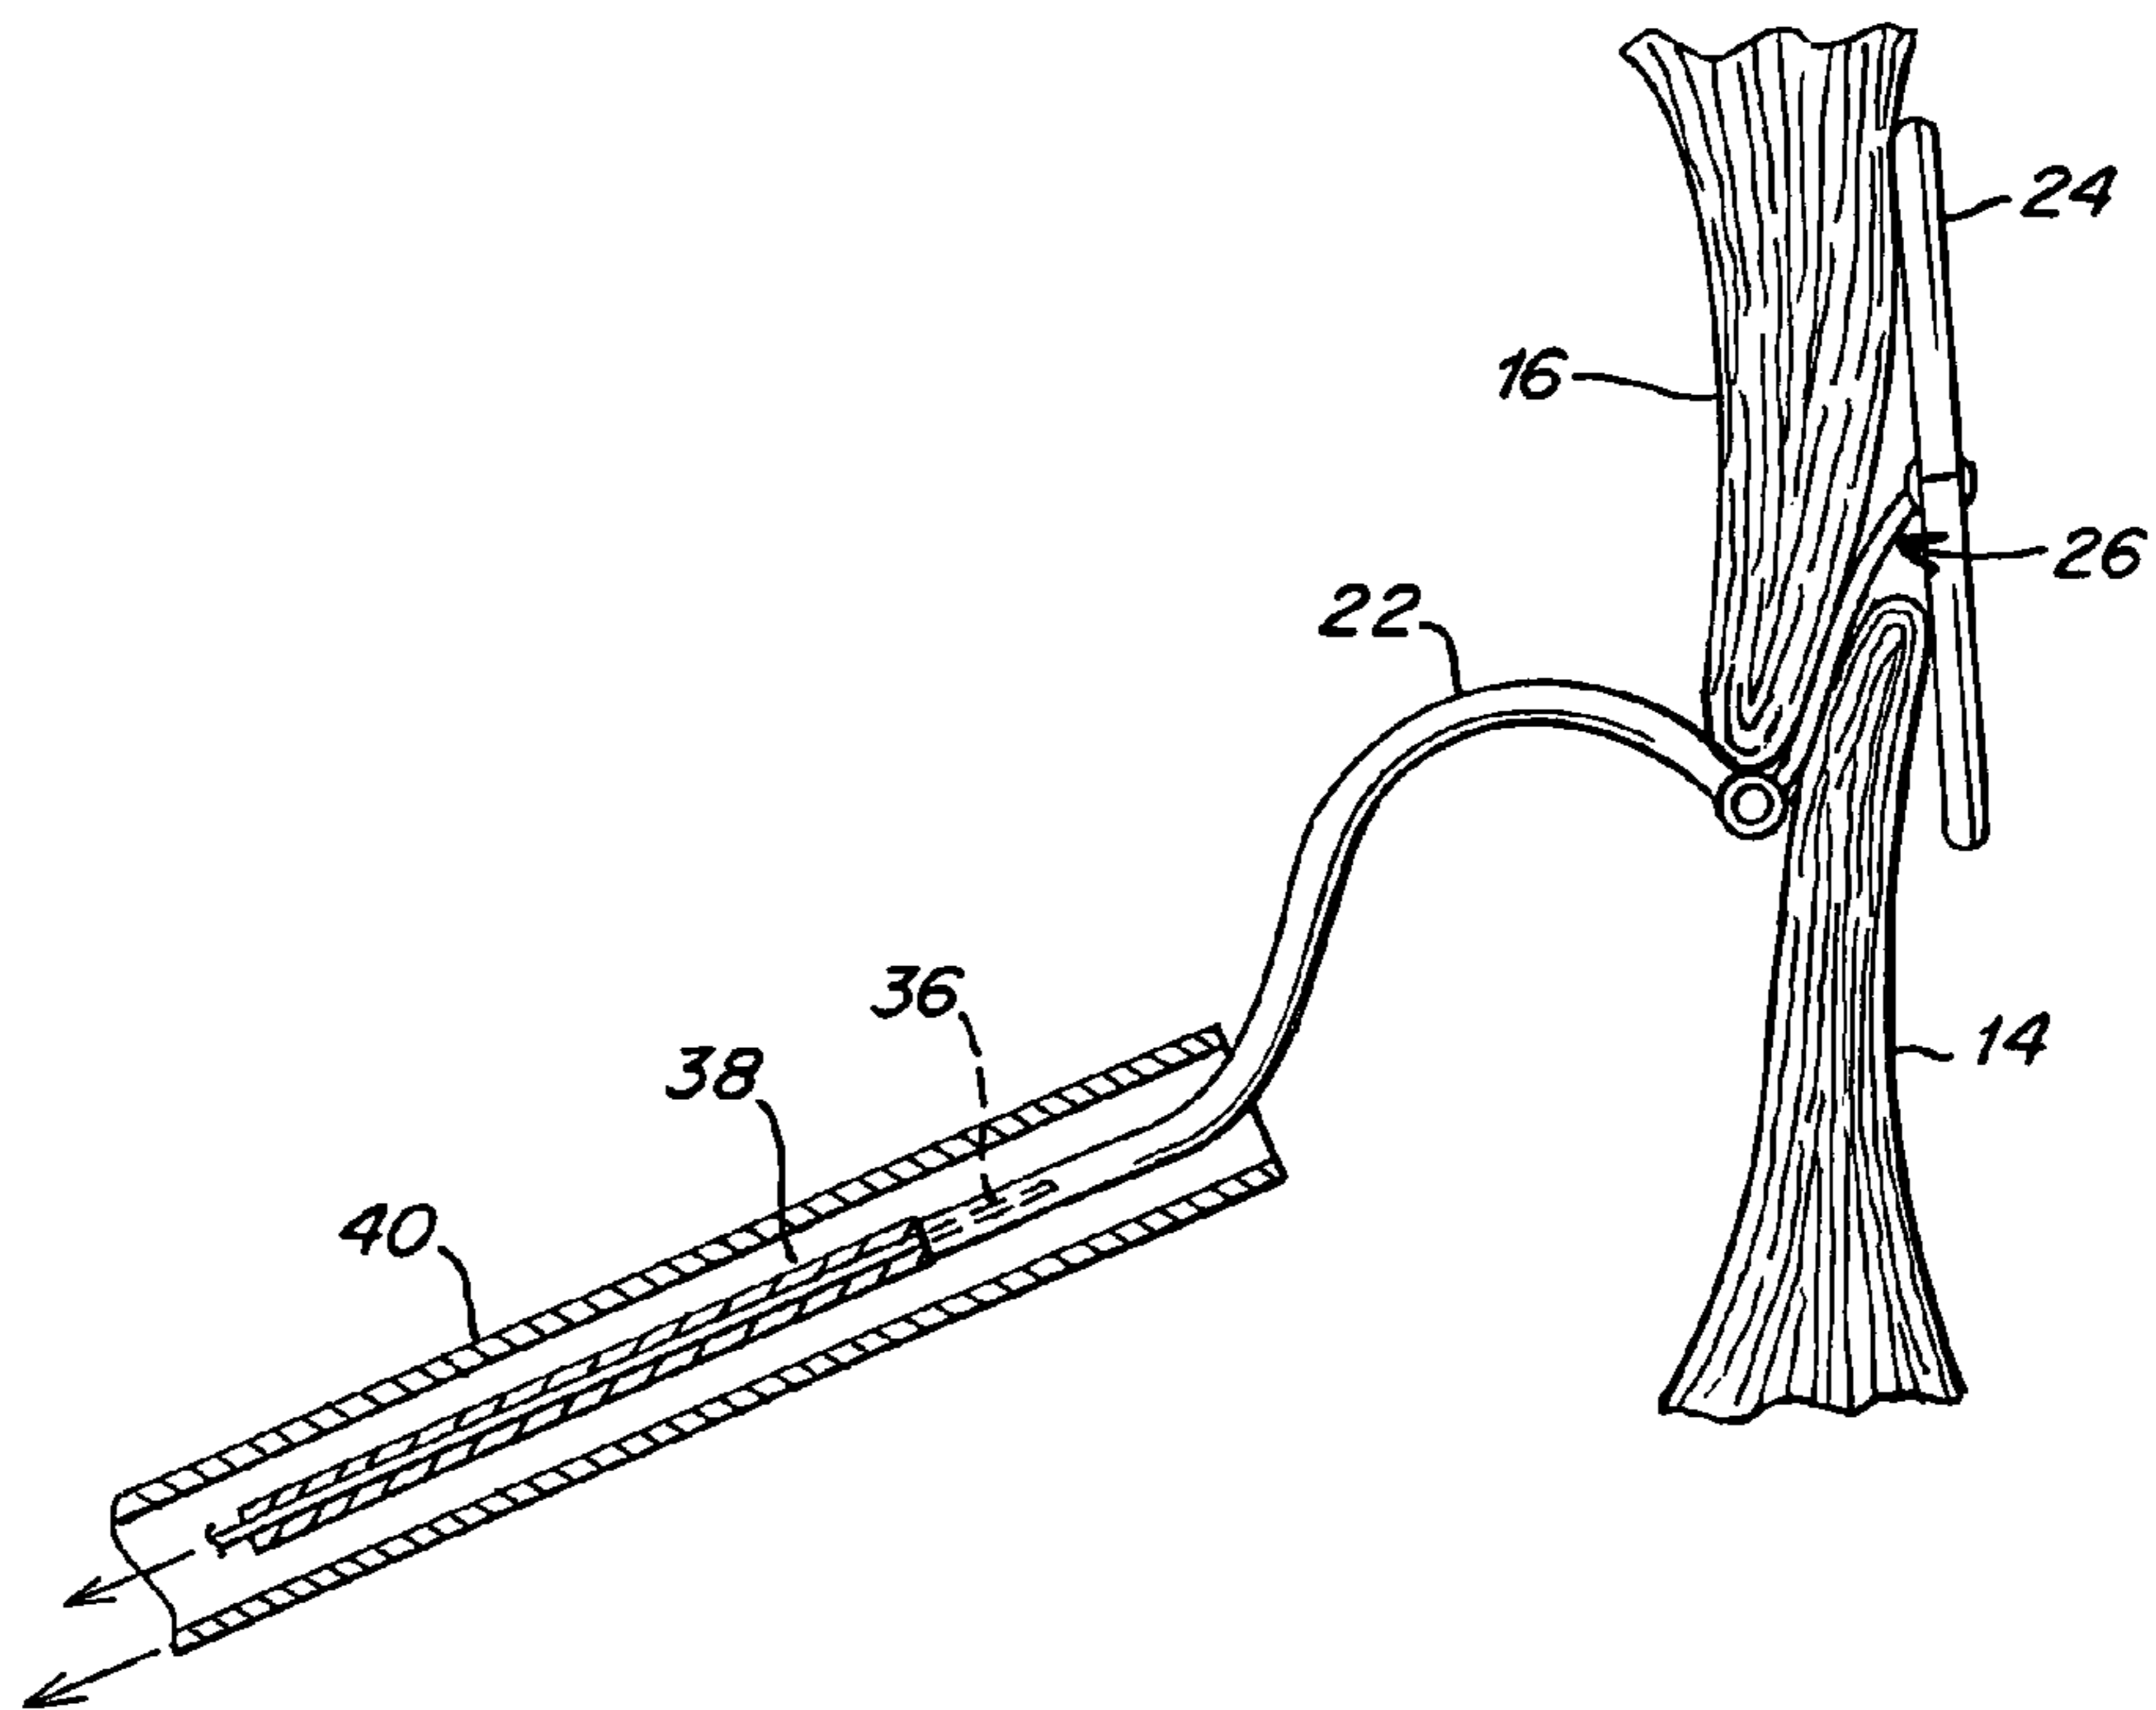


Fig. 8

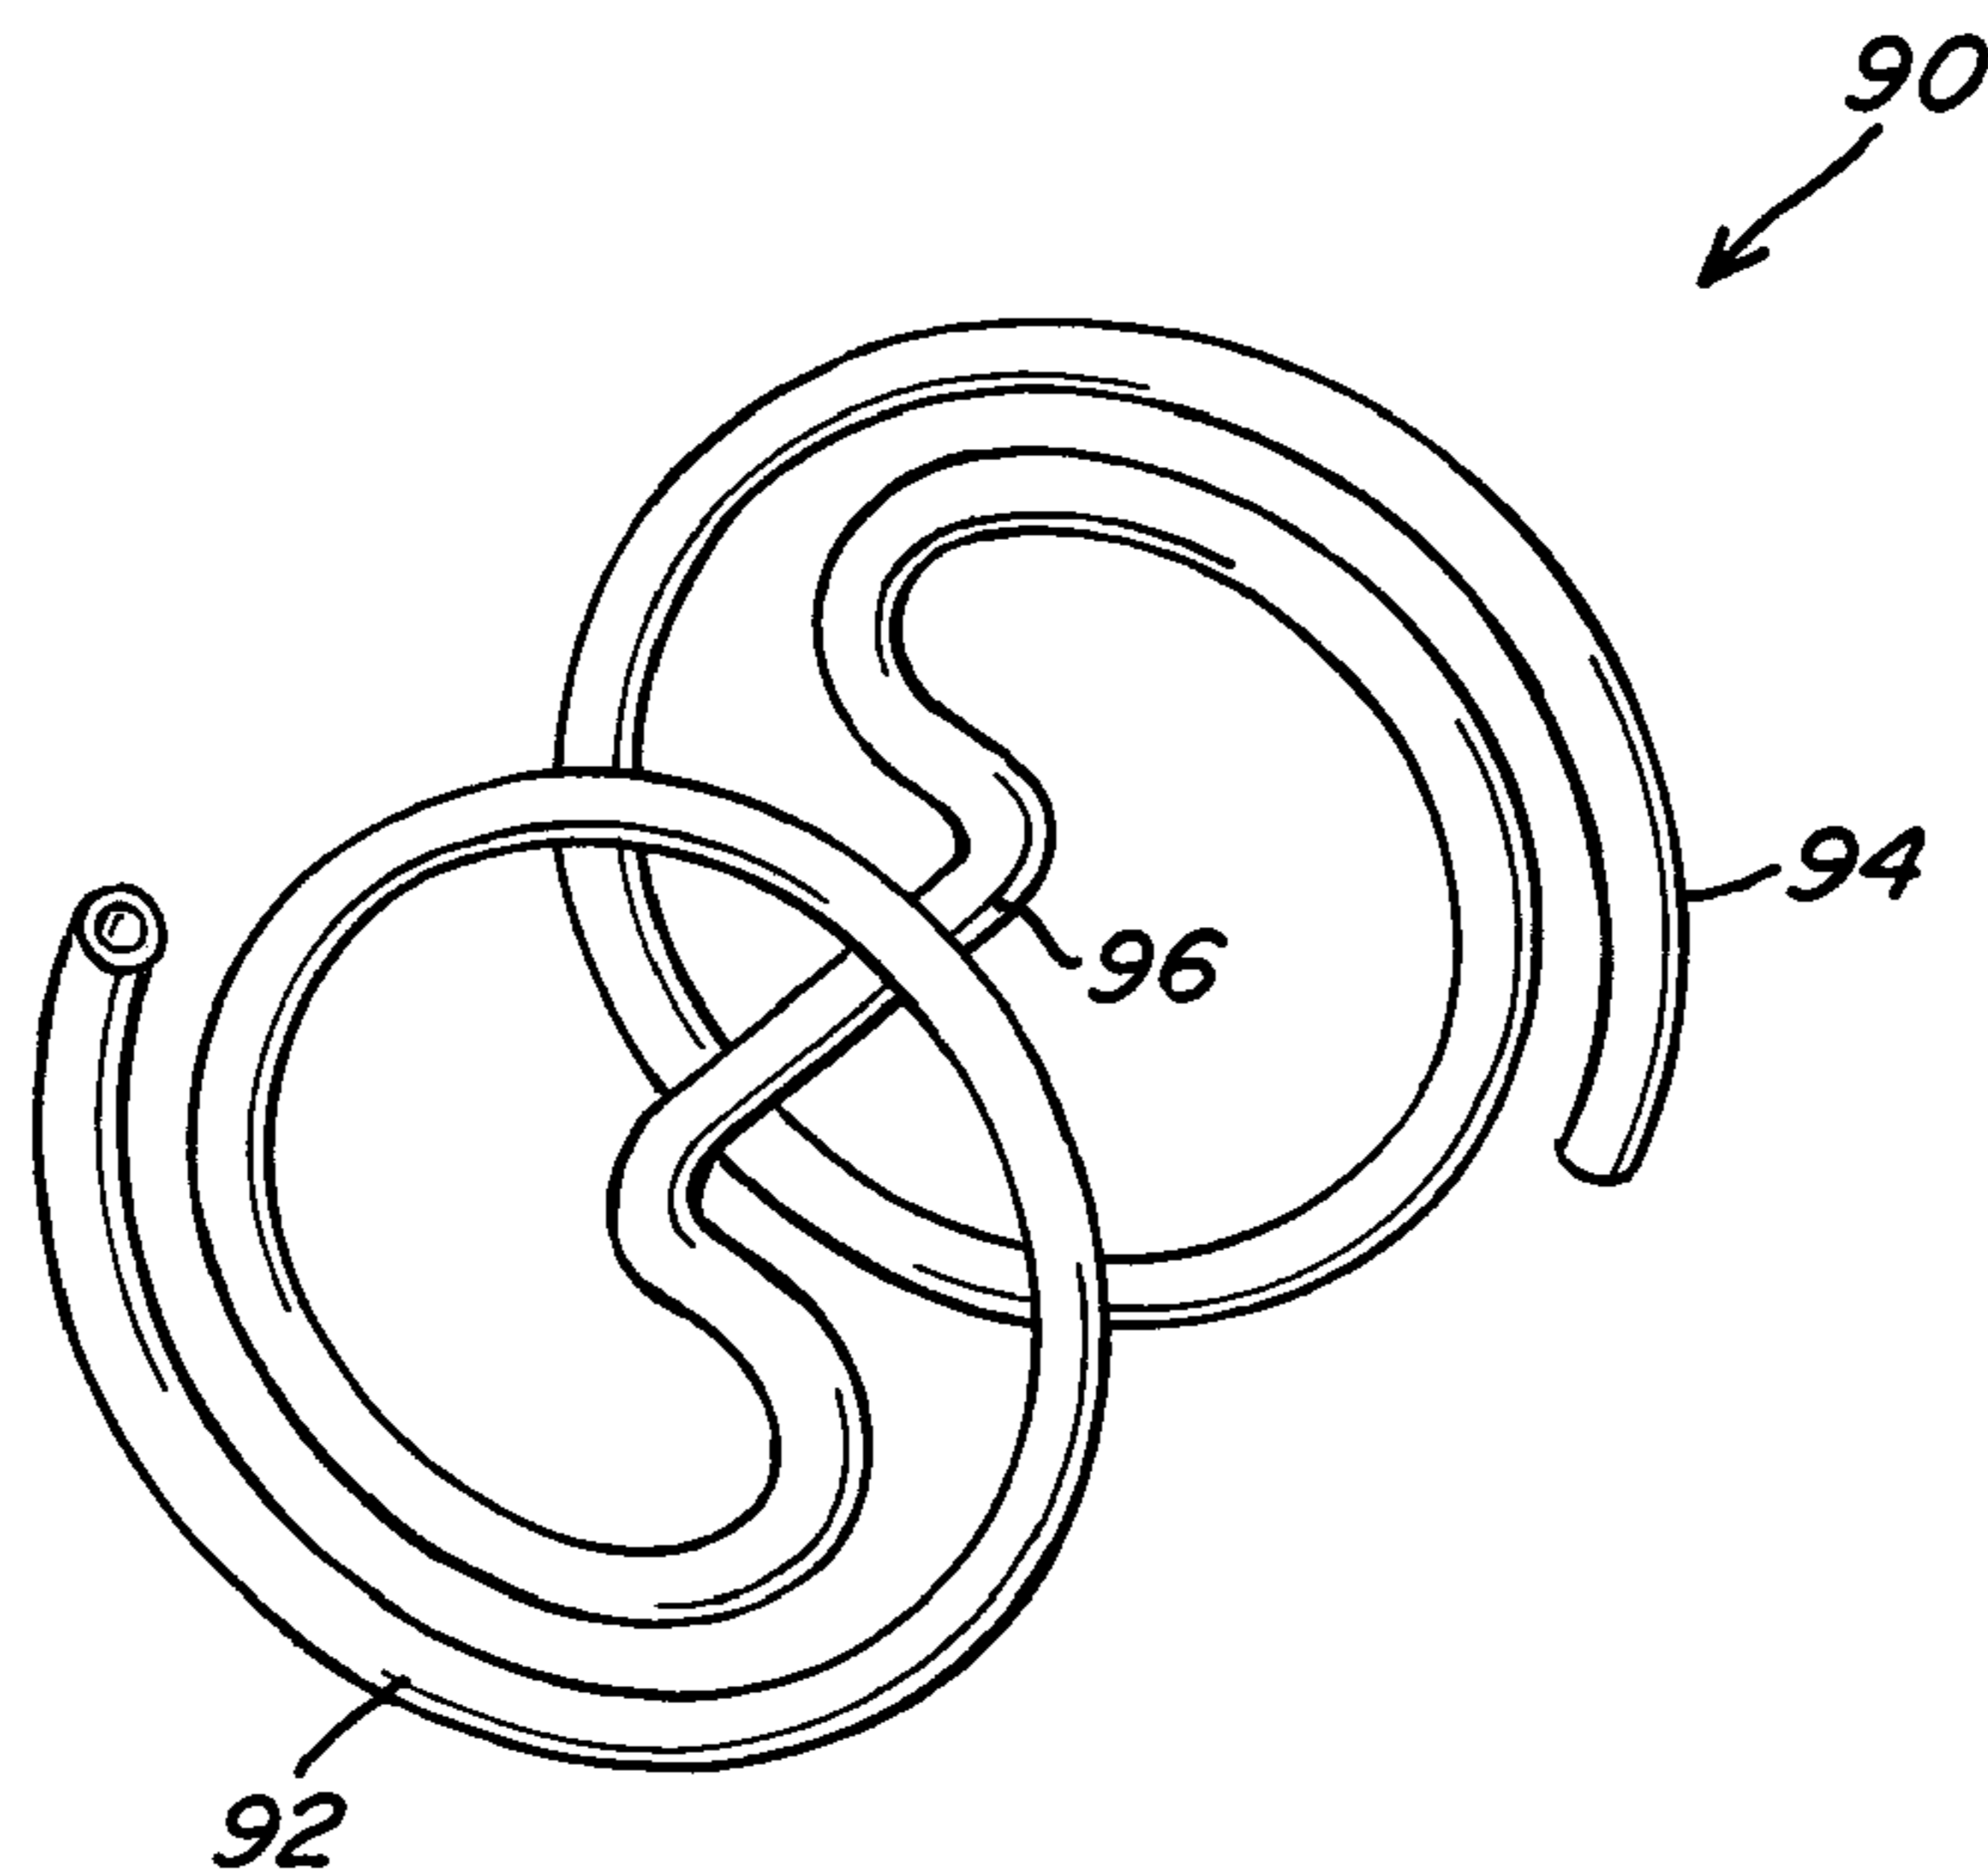


Fig. 9

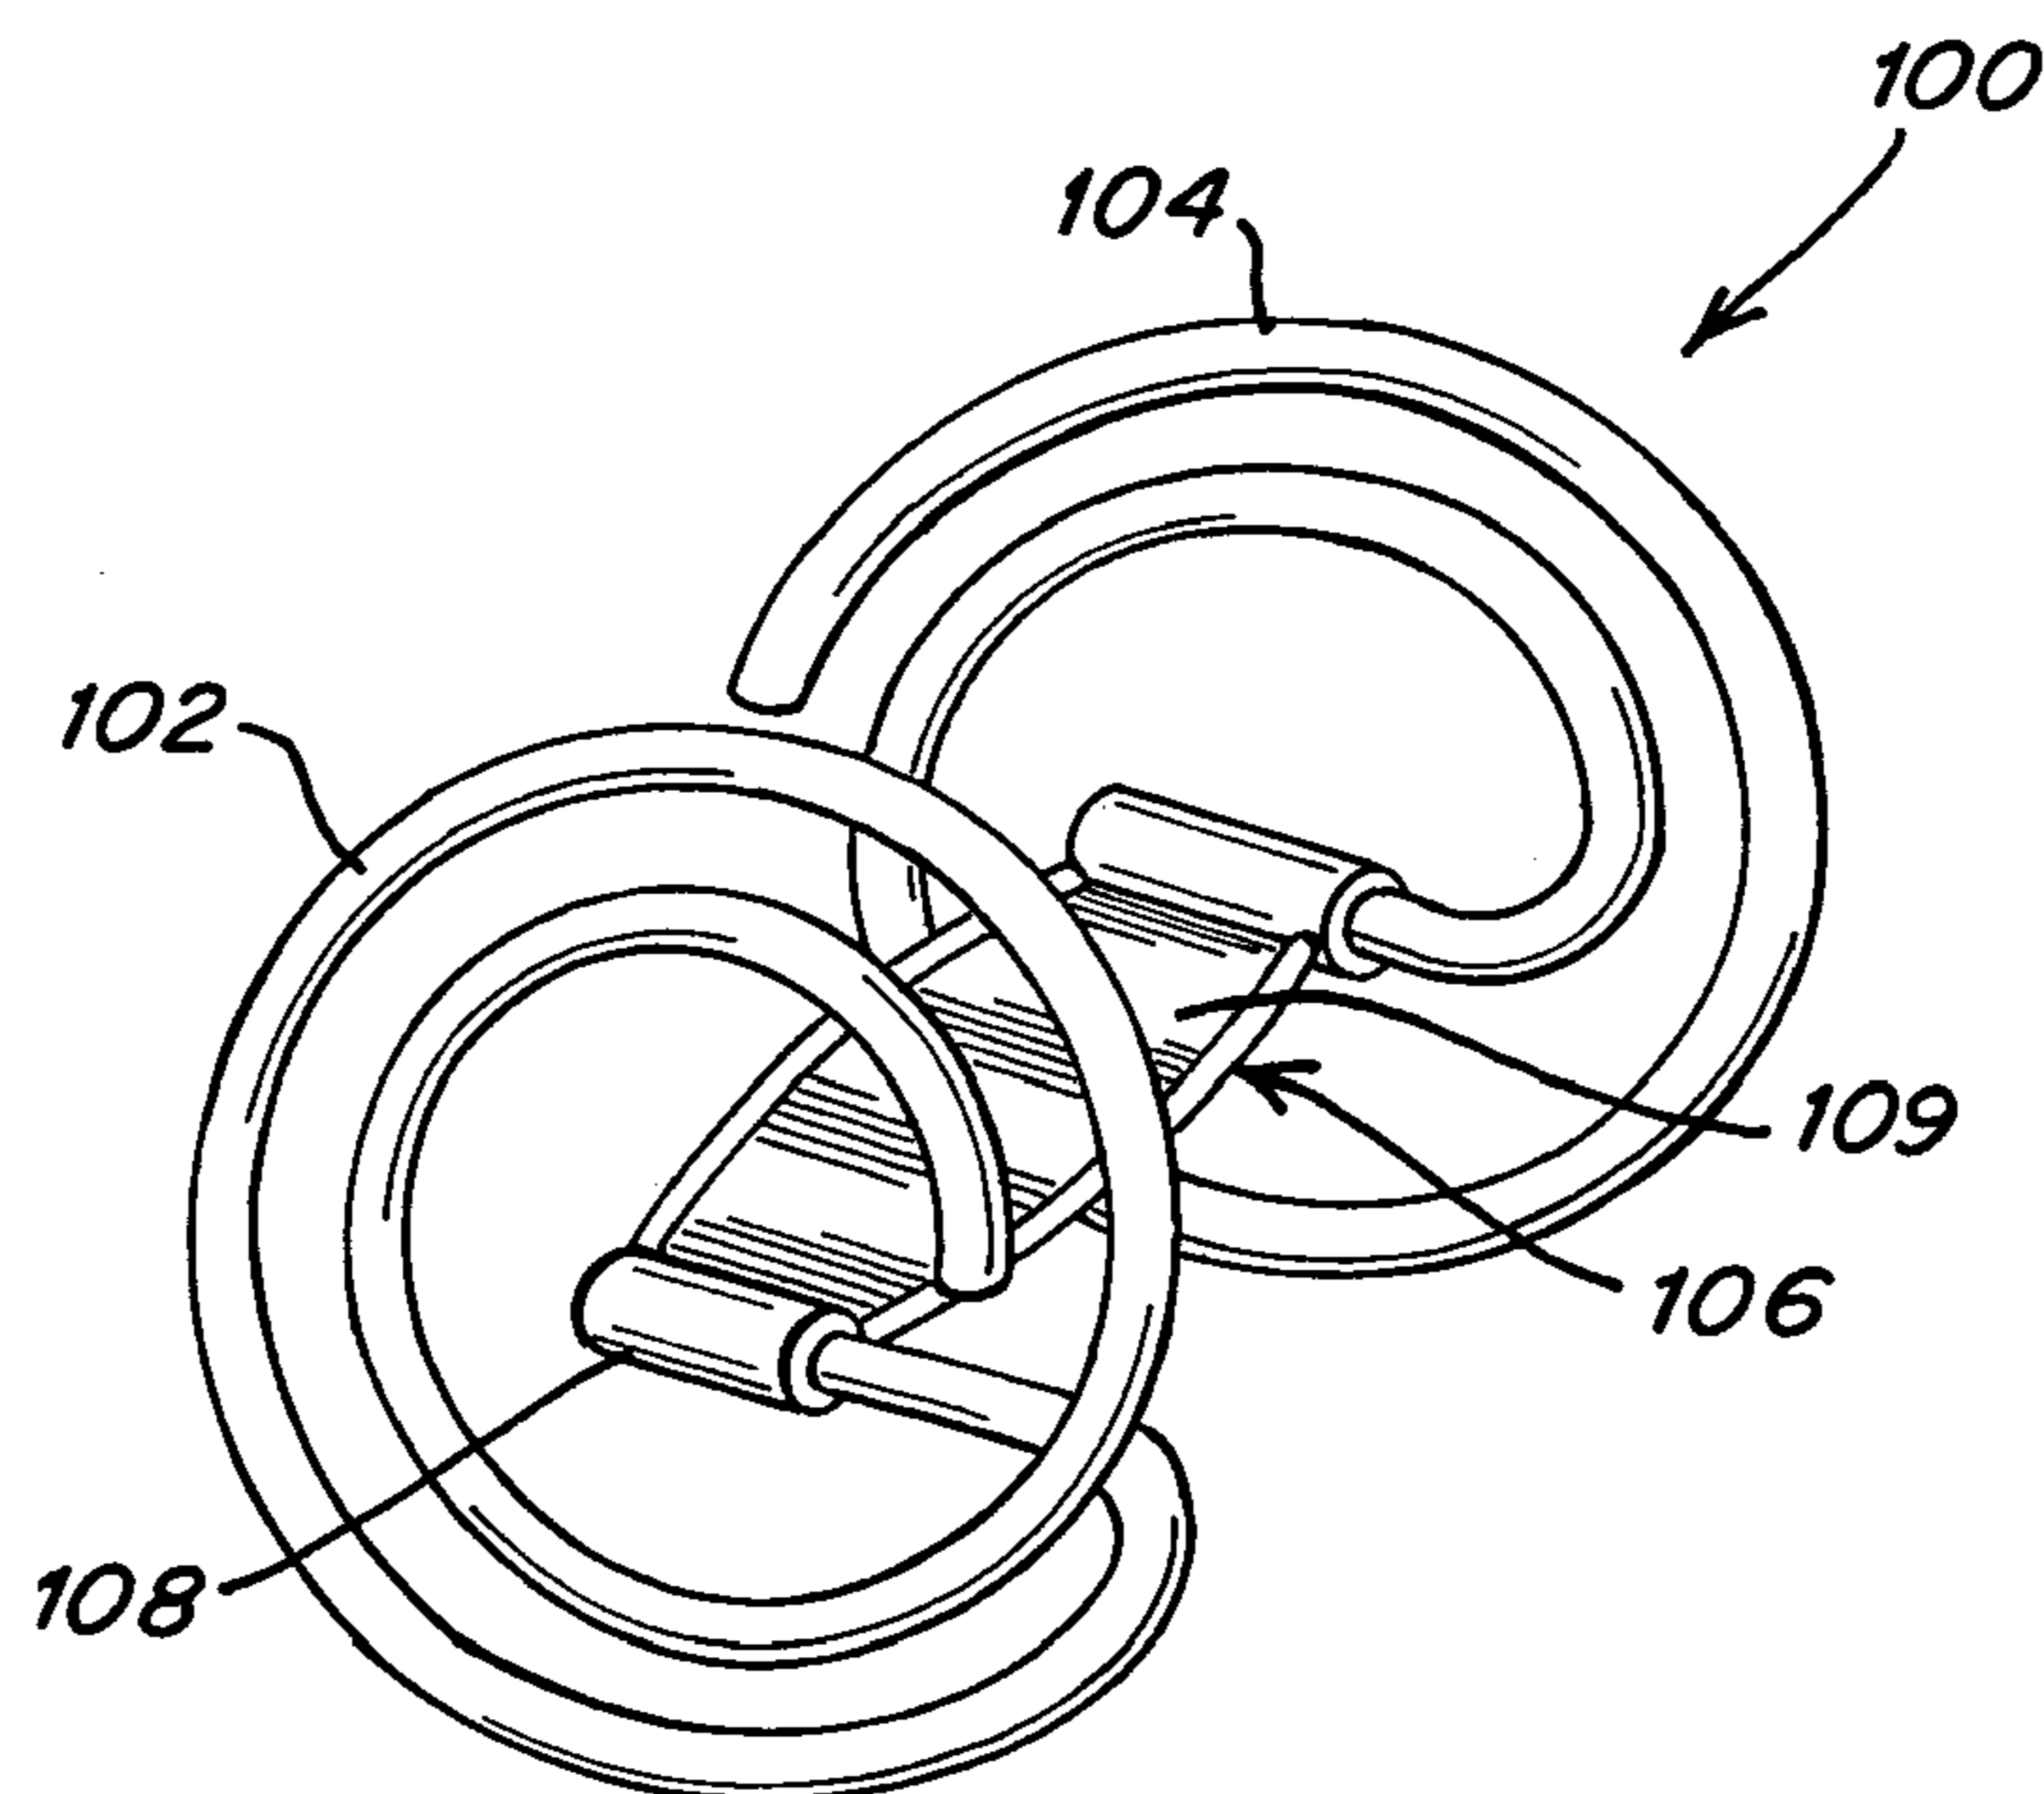


Fig. 10

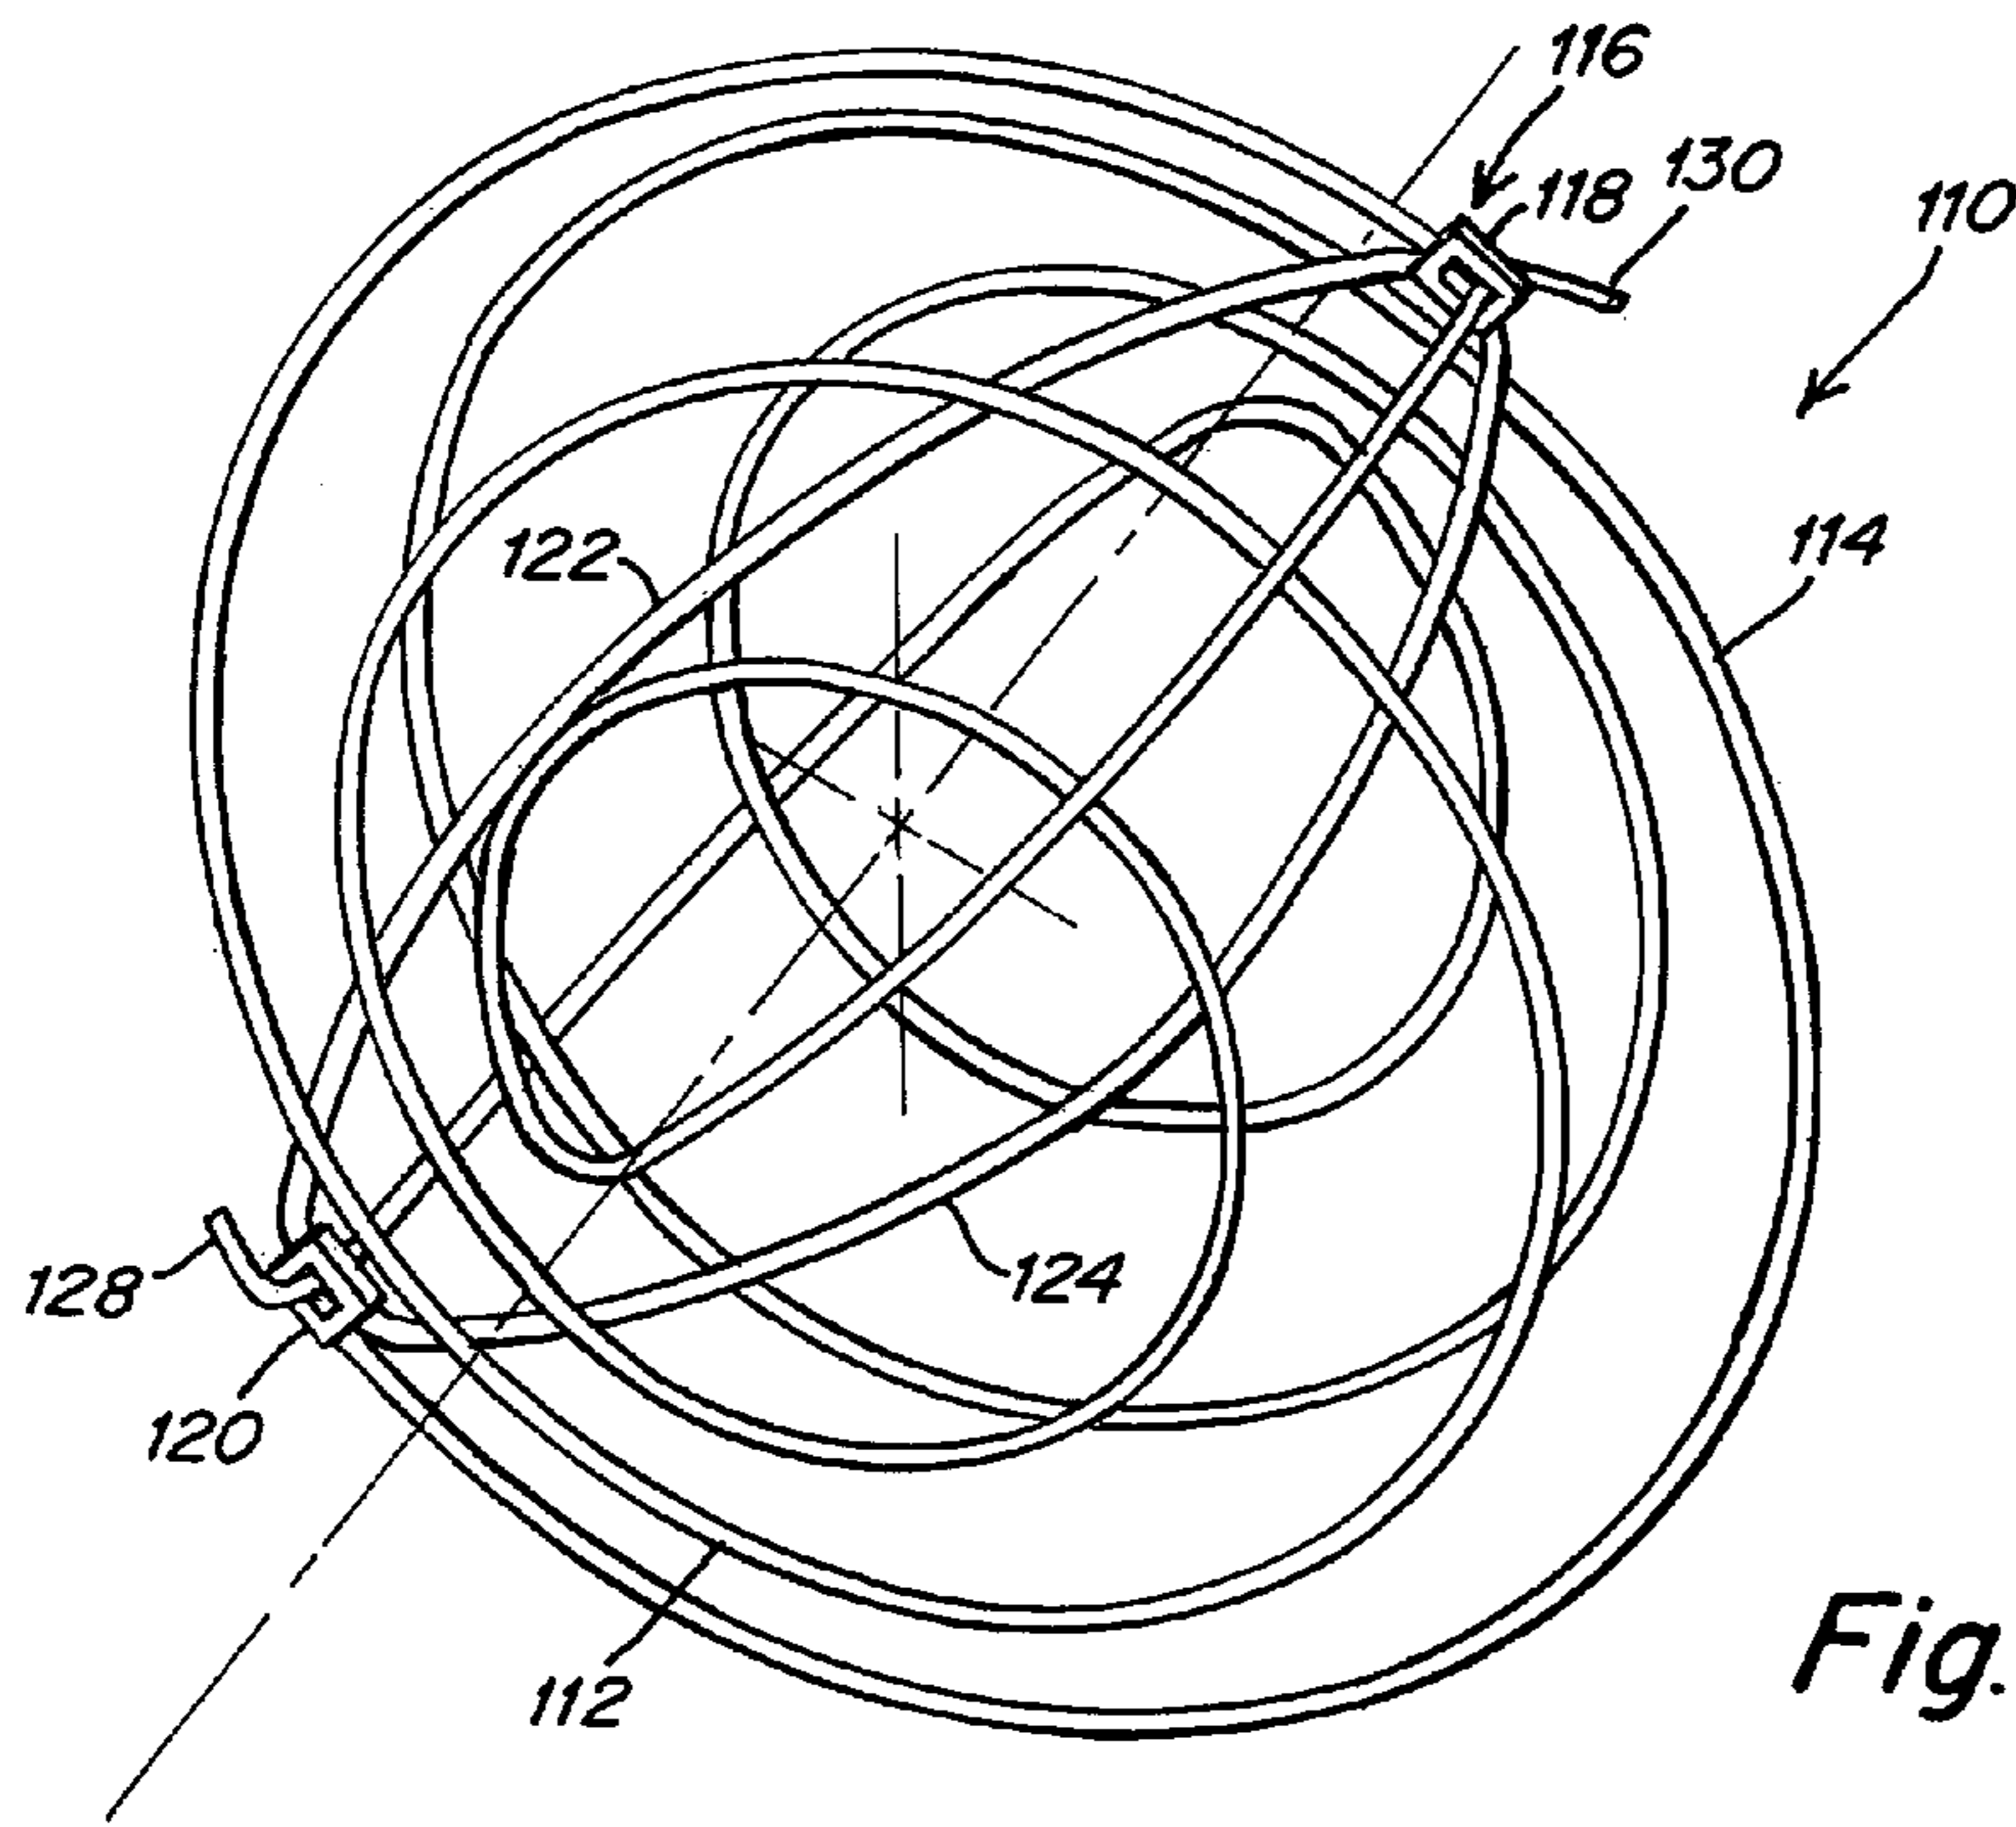


Fig. 11

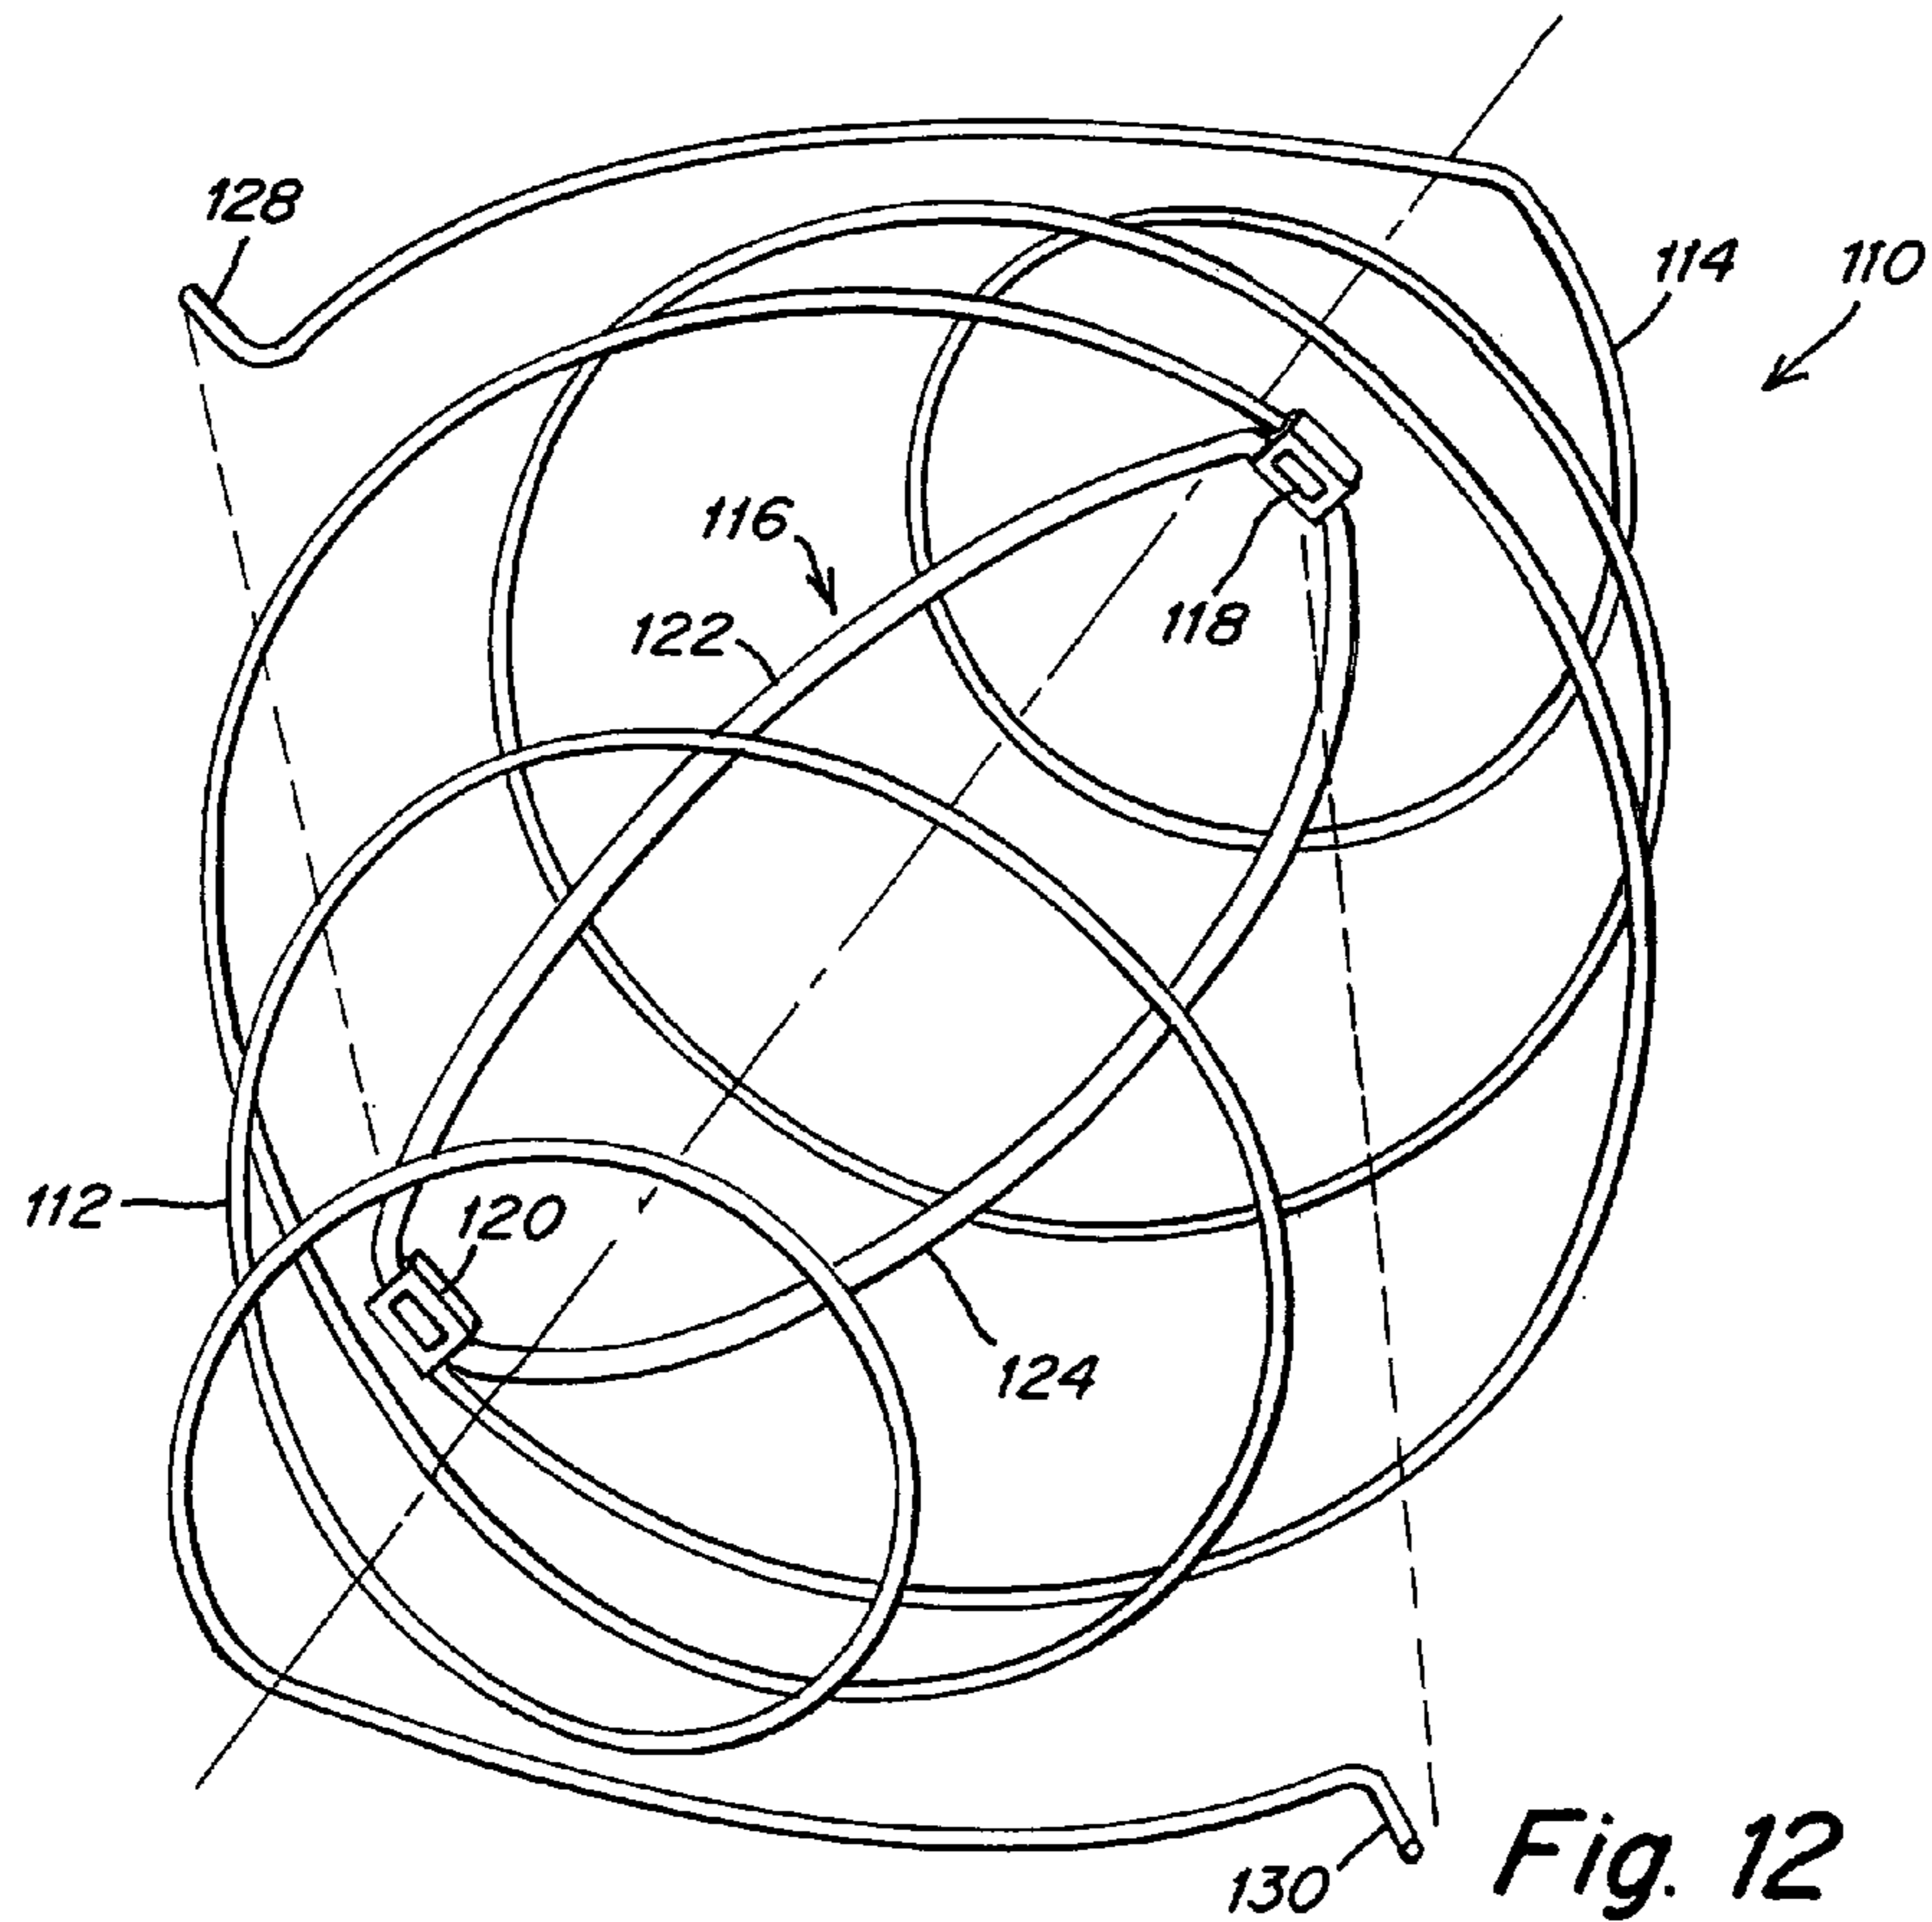


Fig. 12

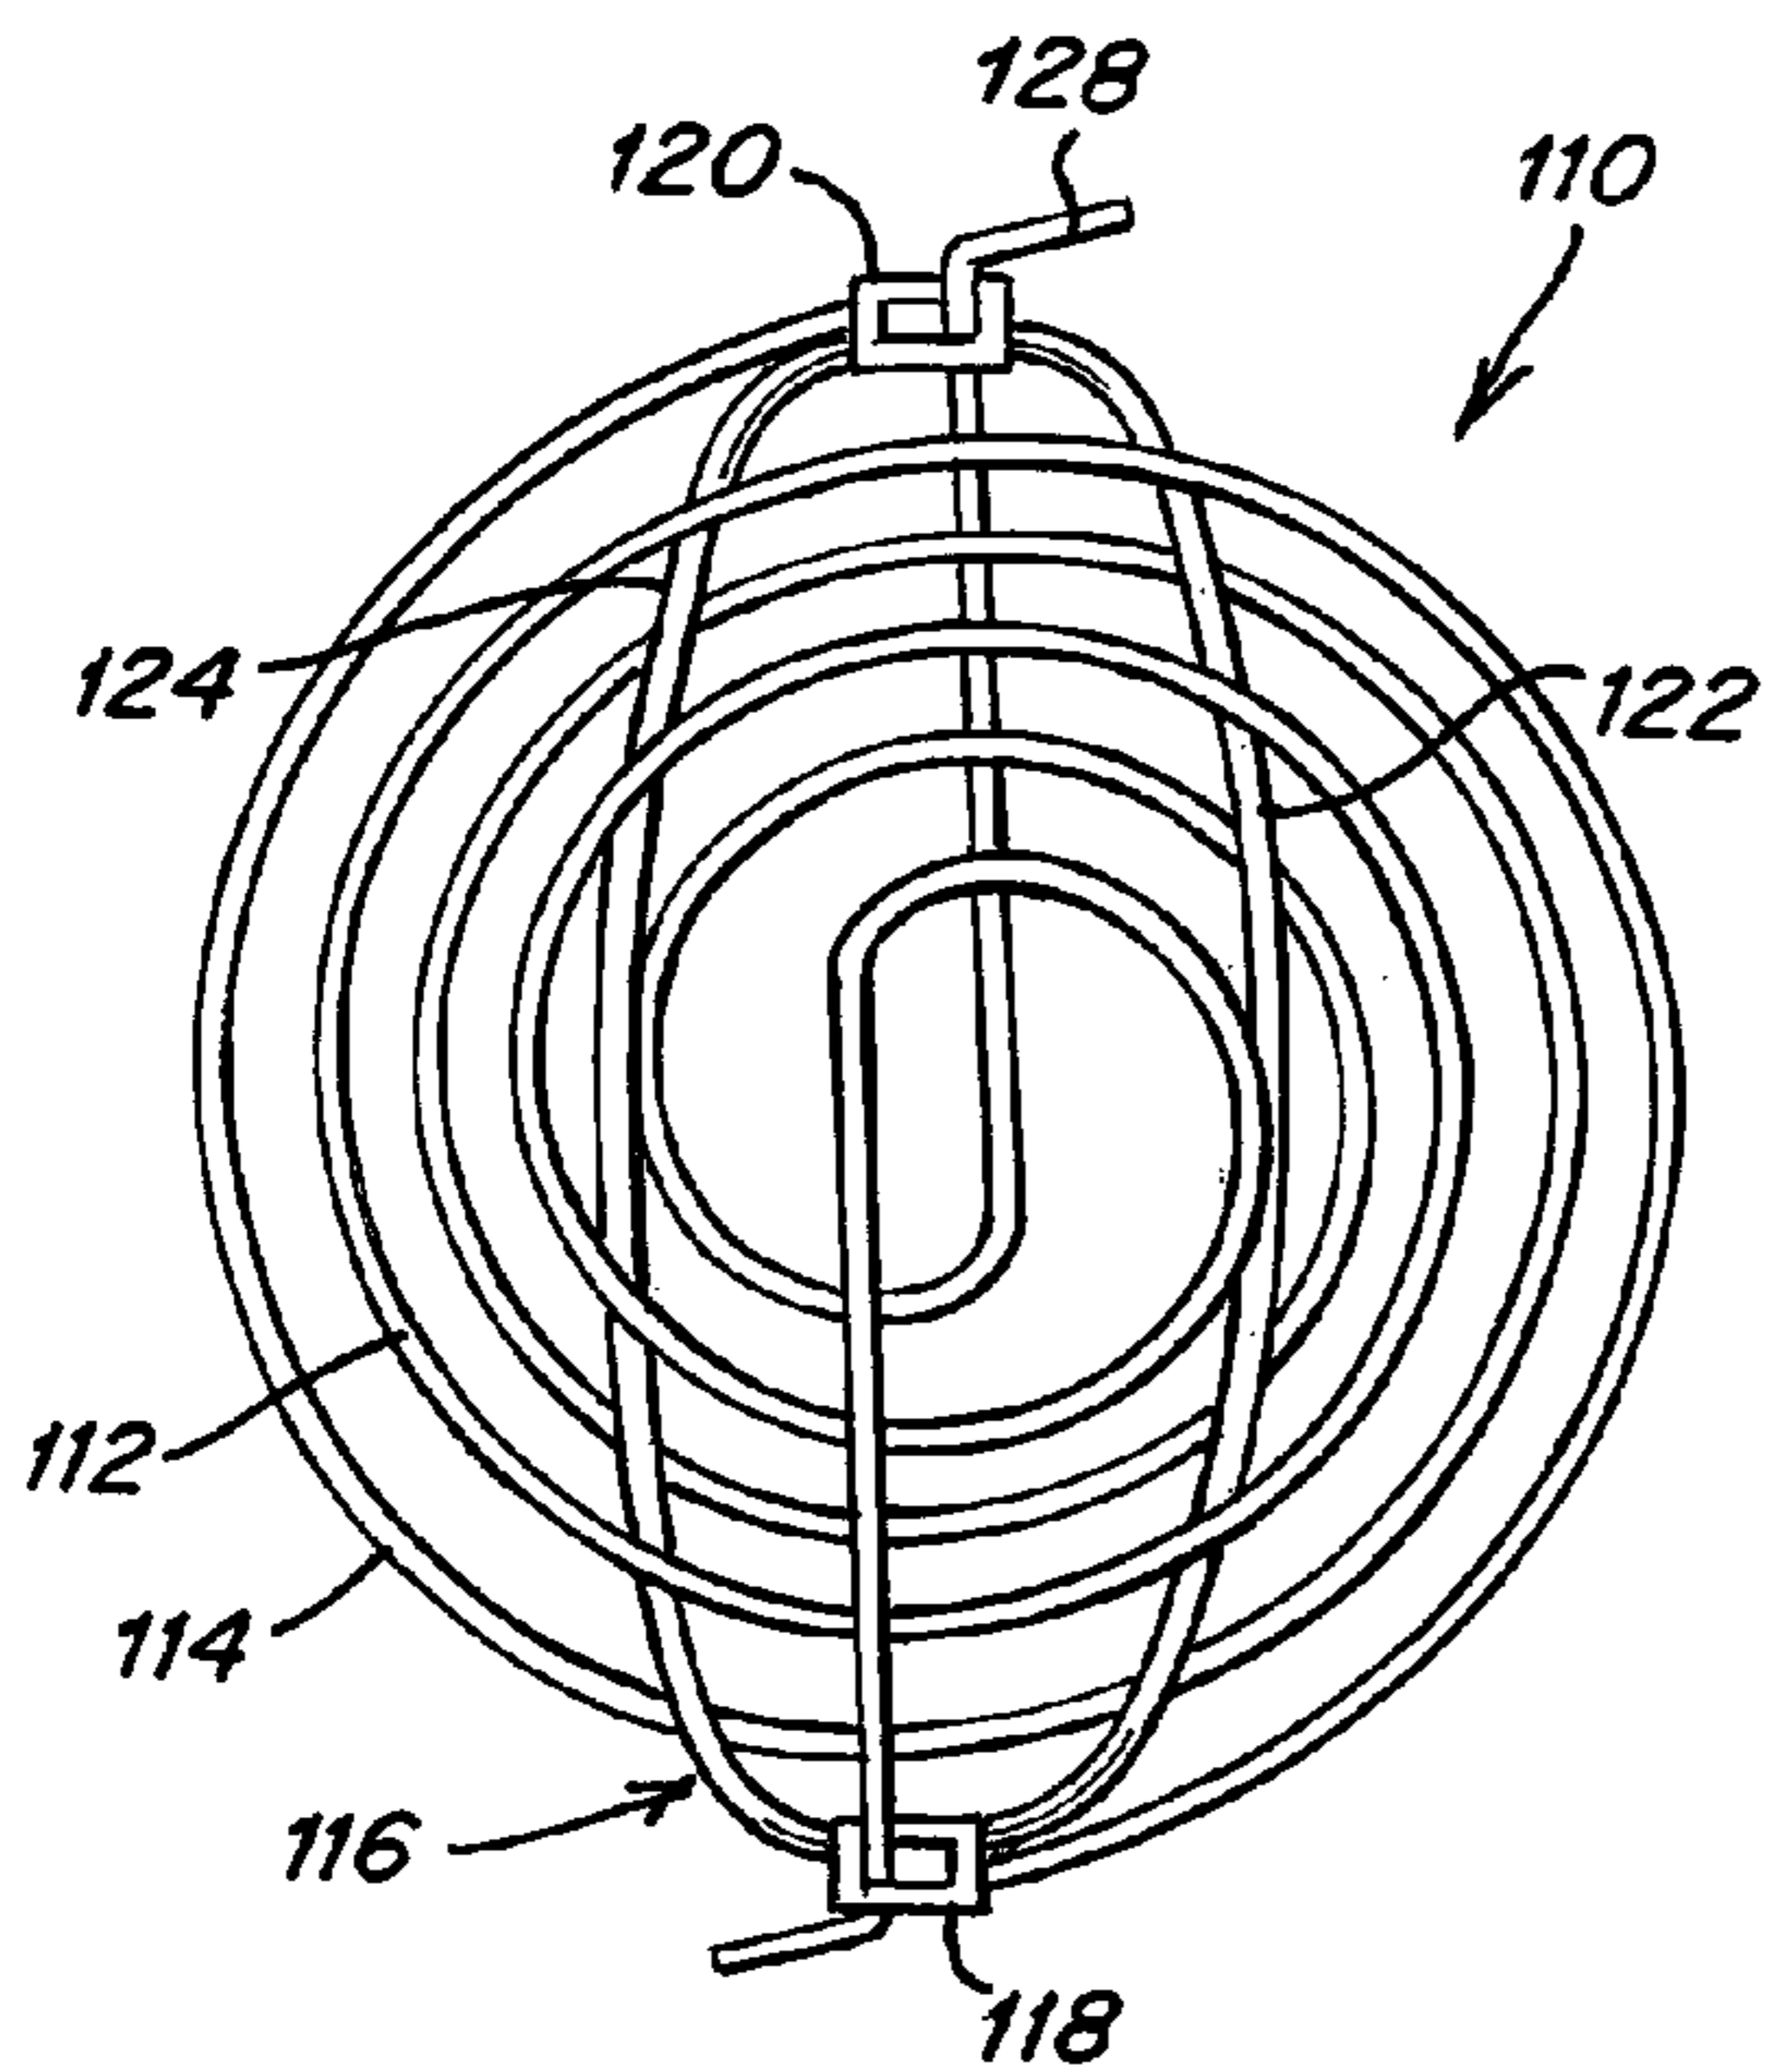


Fig. 13

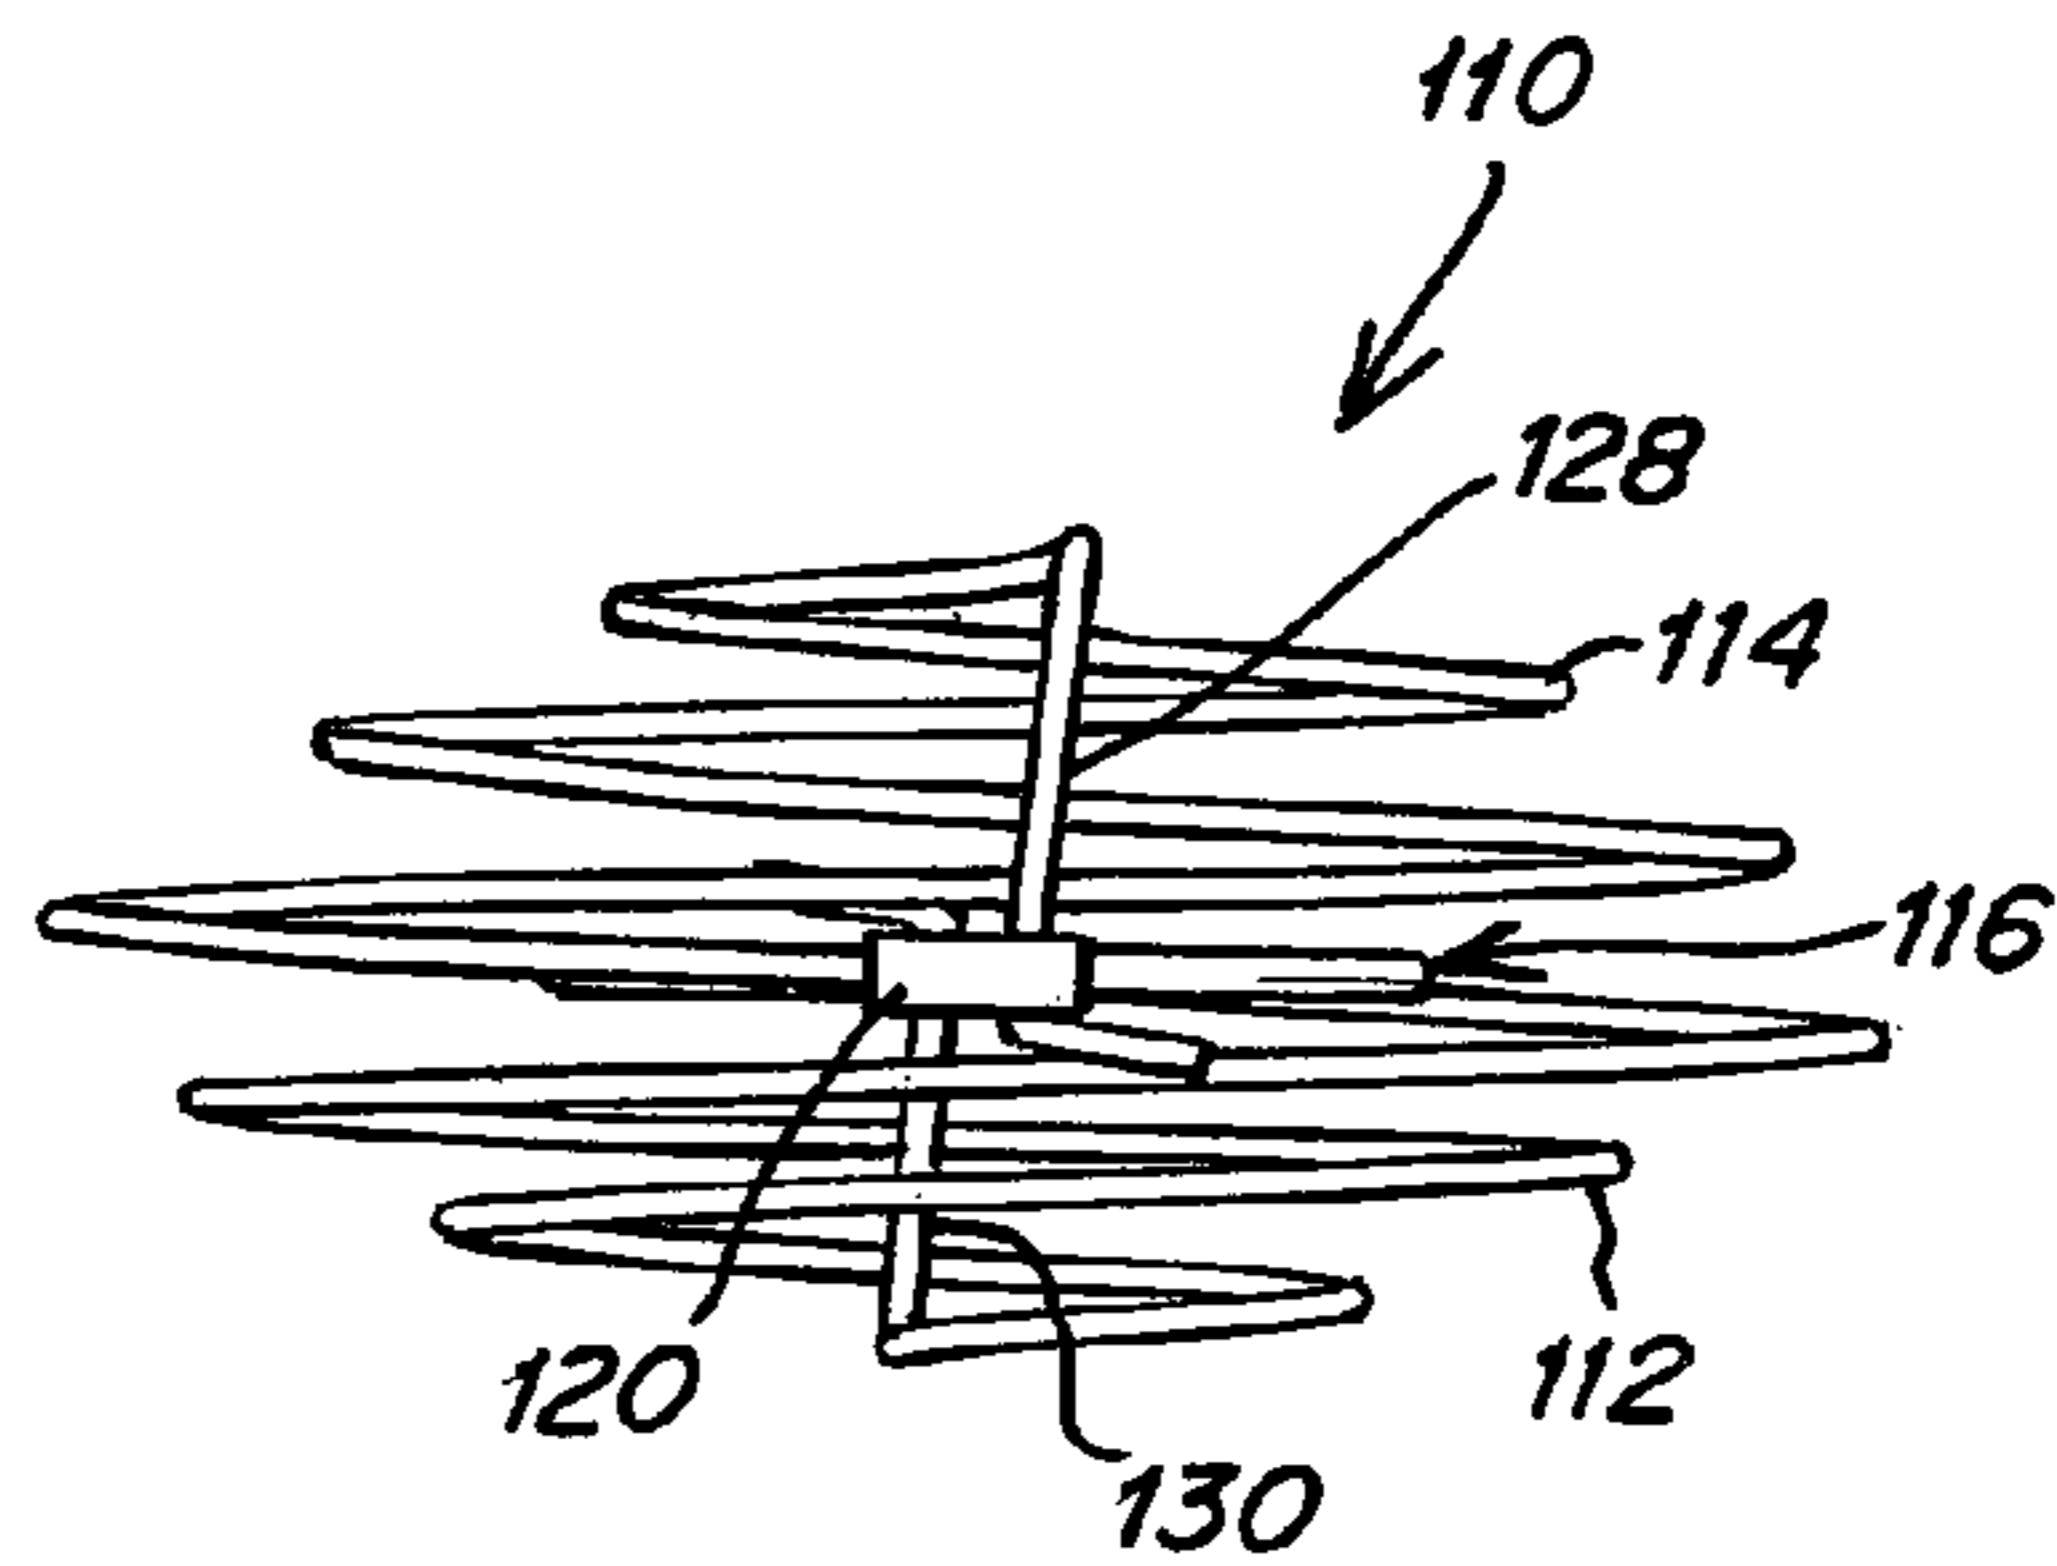


Fig. 14

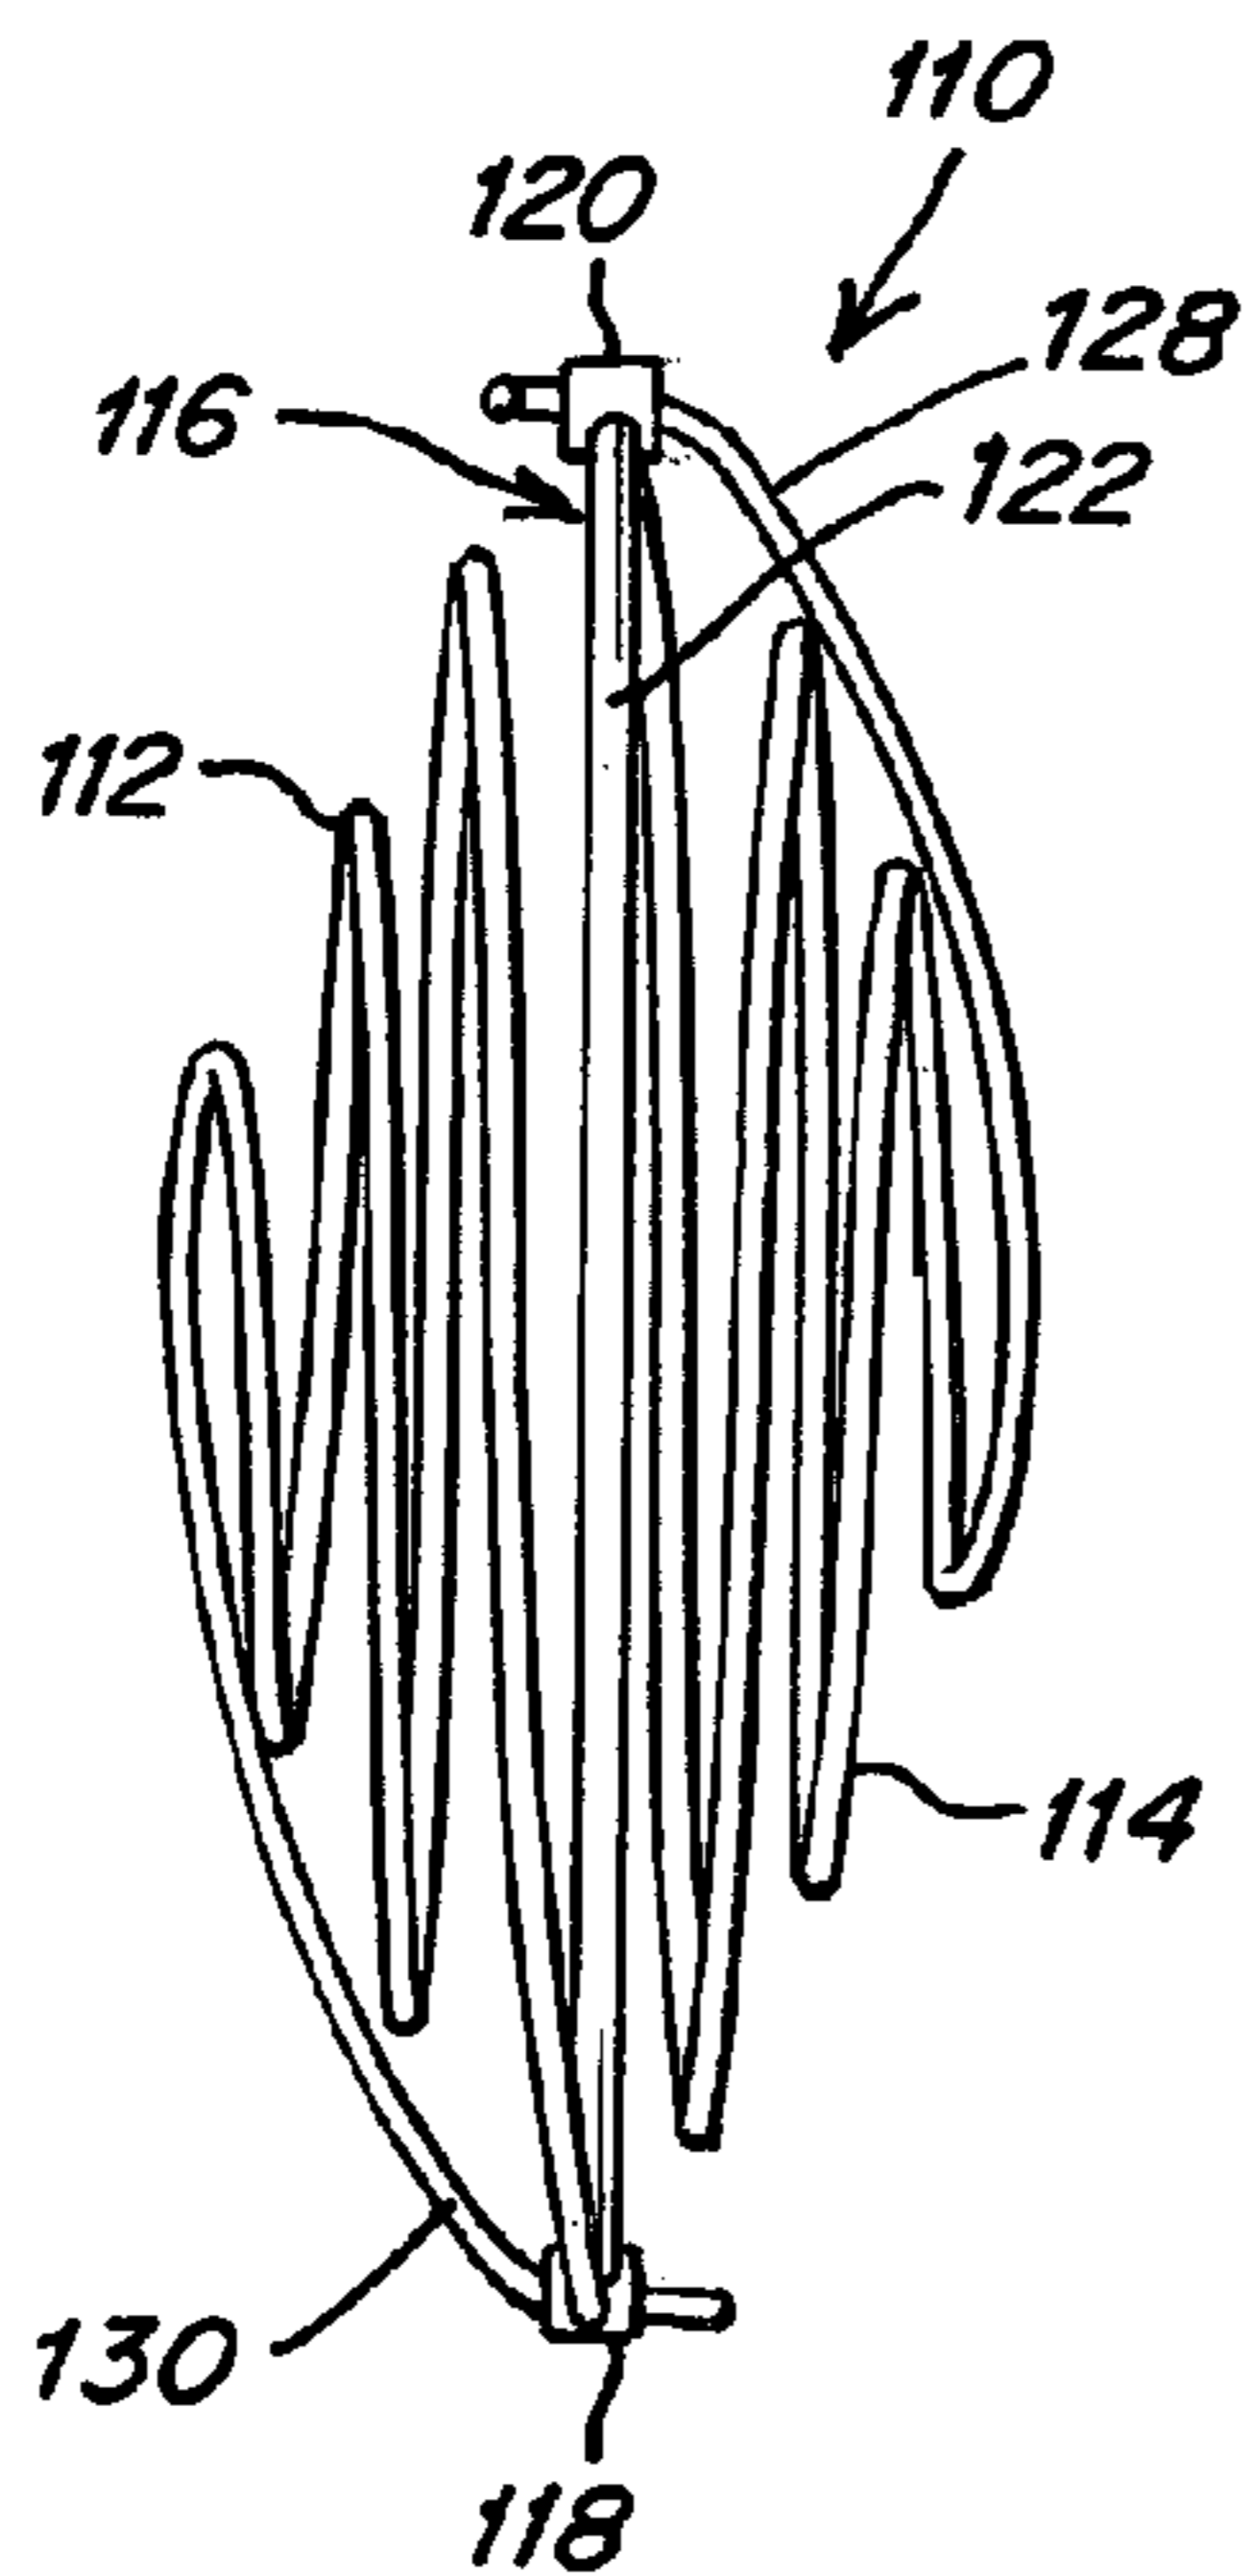


Fig. 15

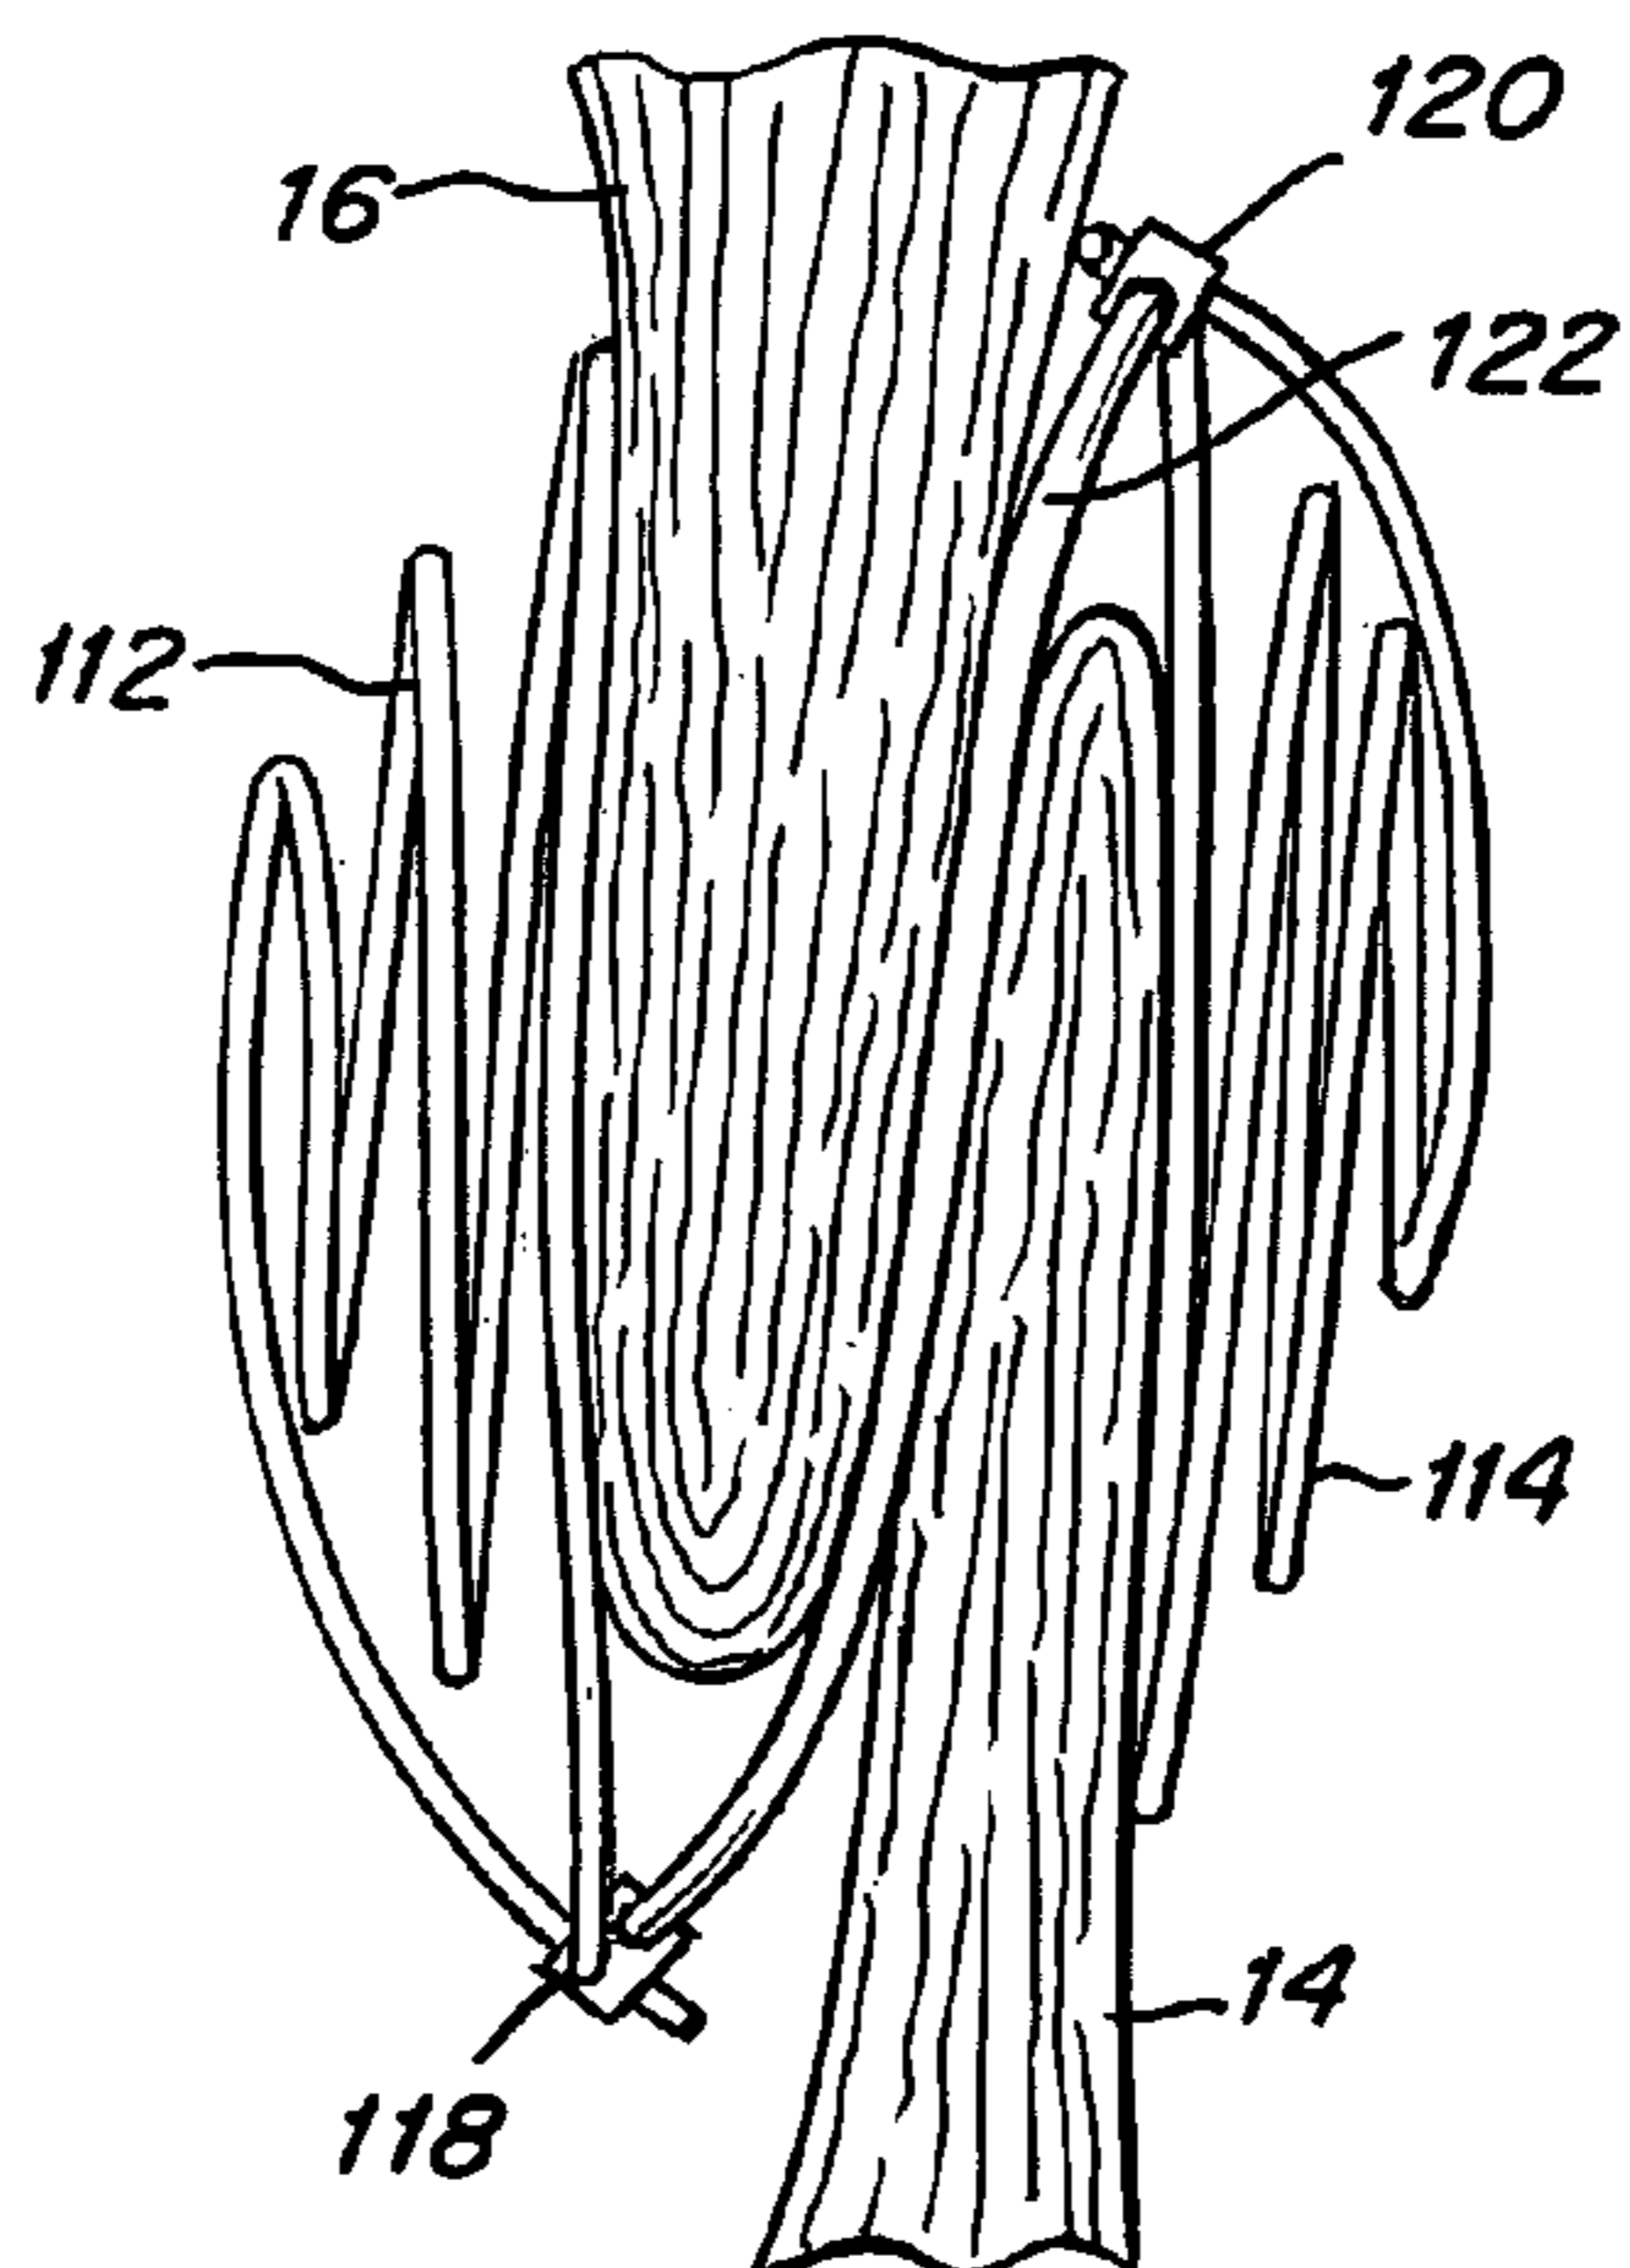


Fig. 16

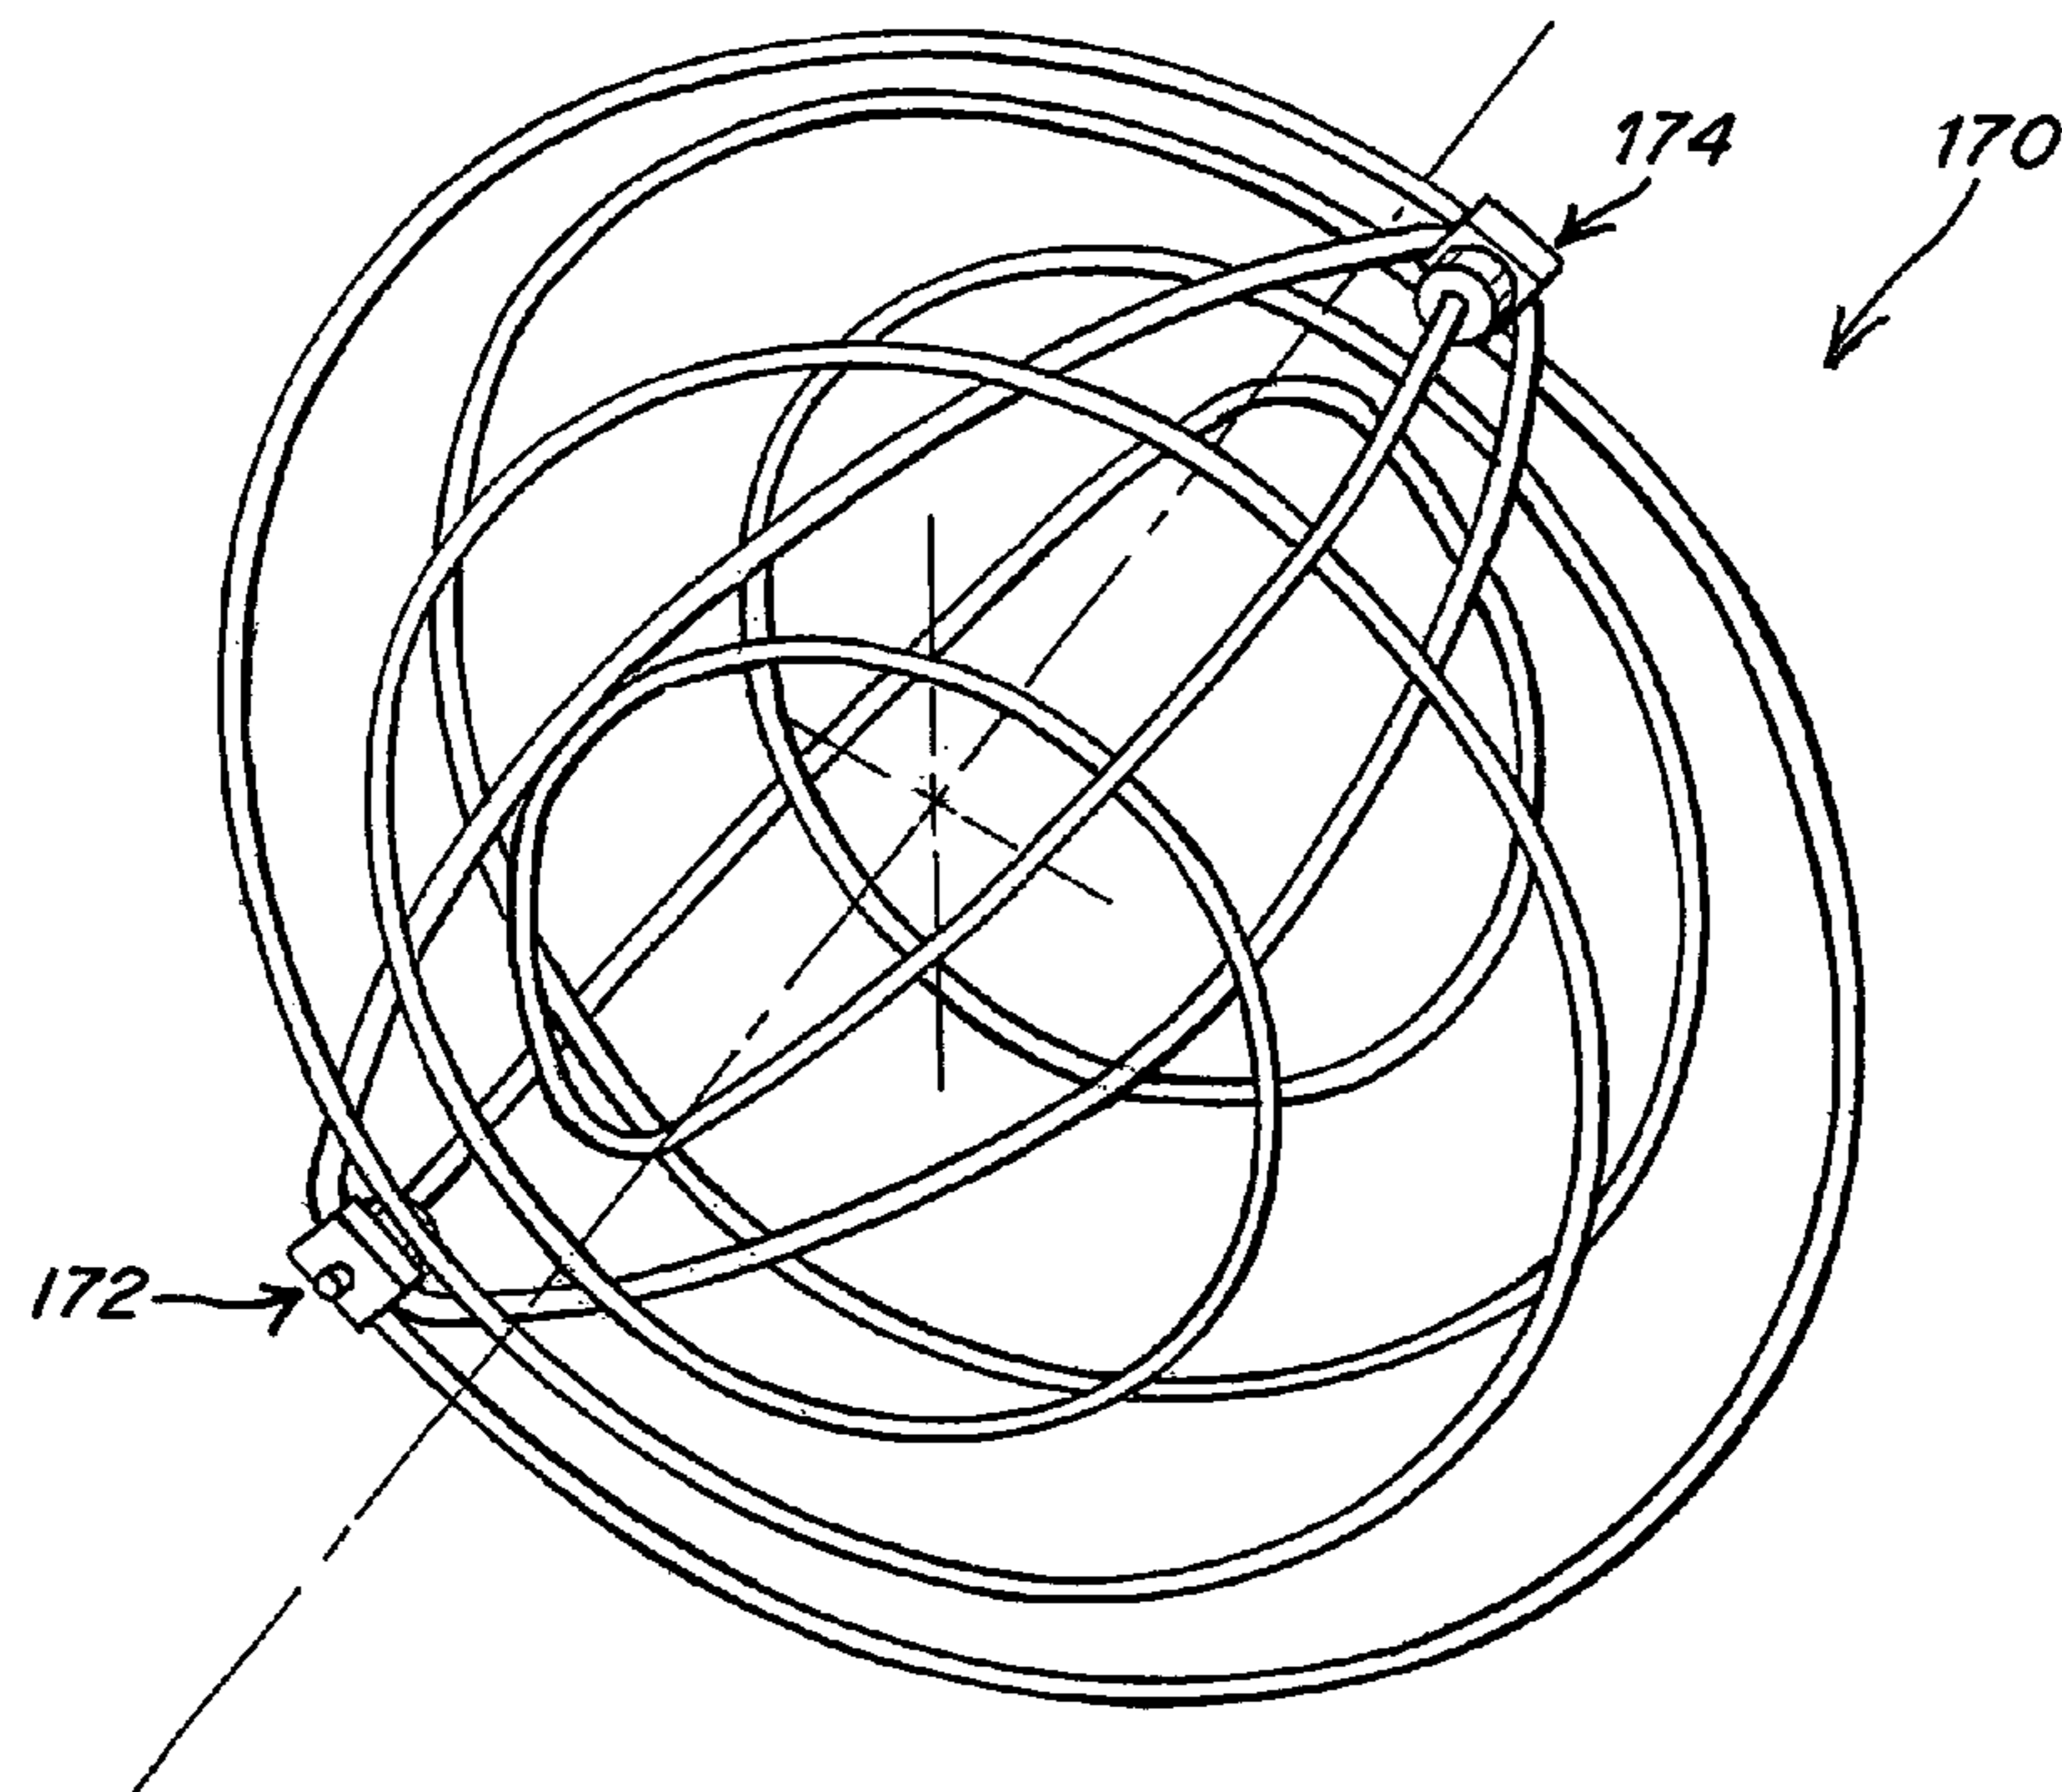


Fig. 17

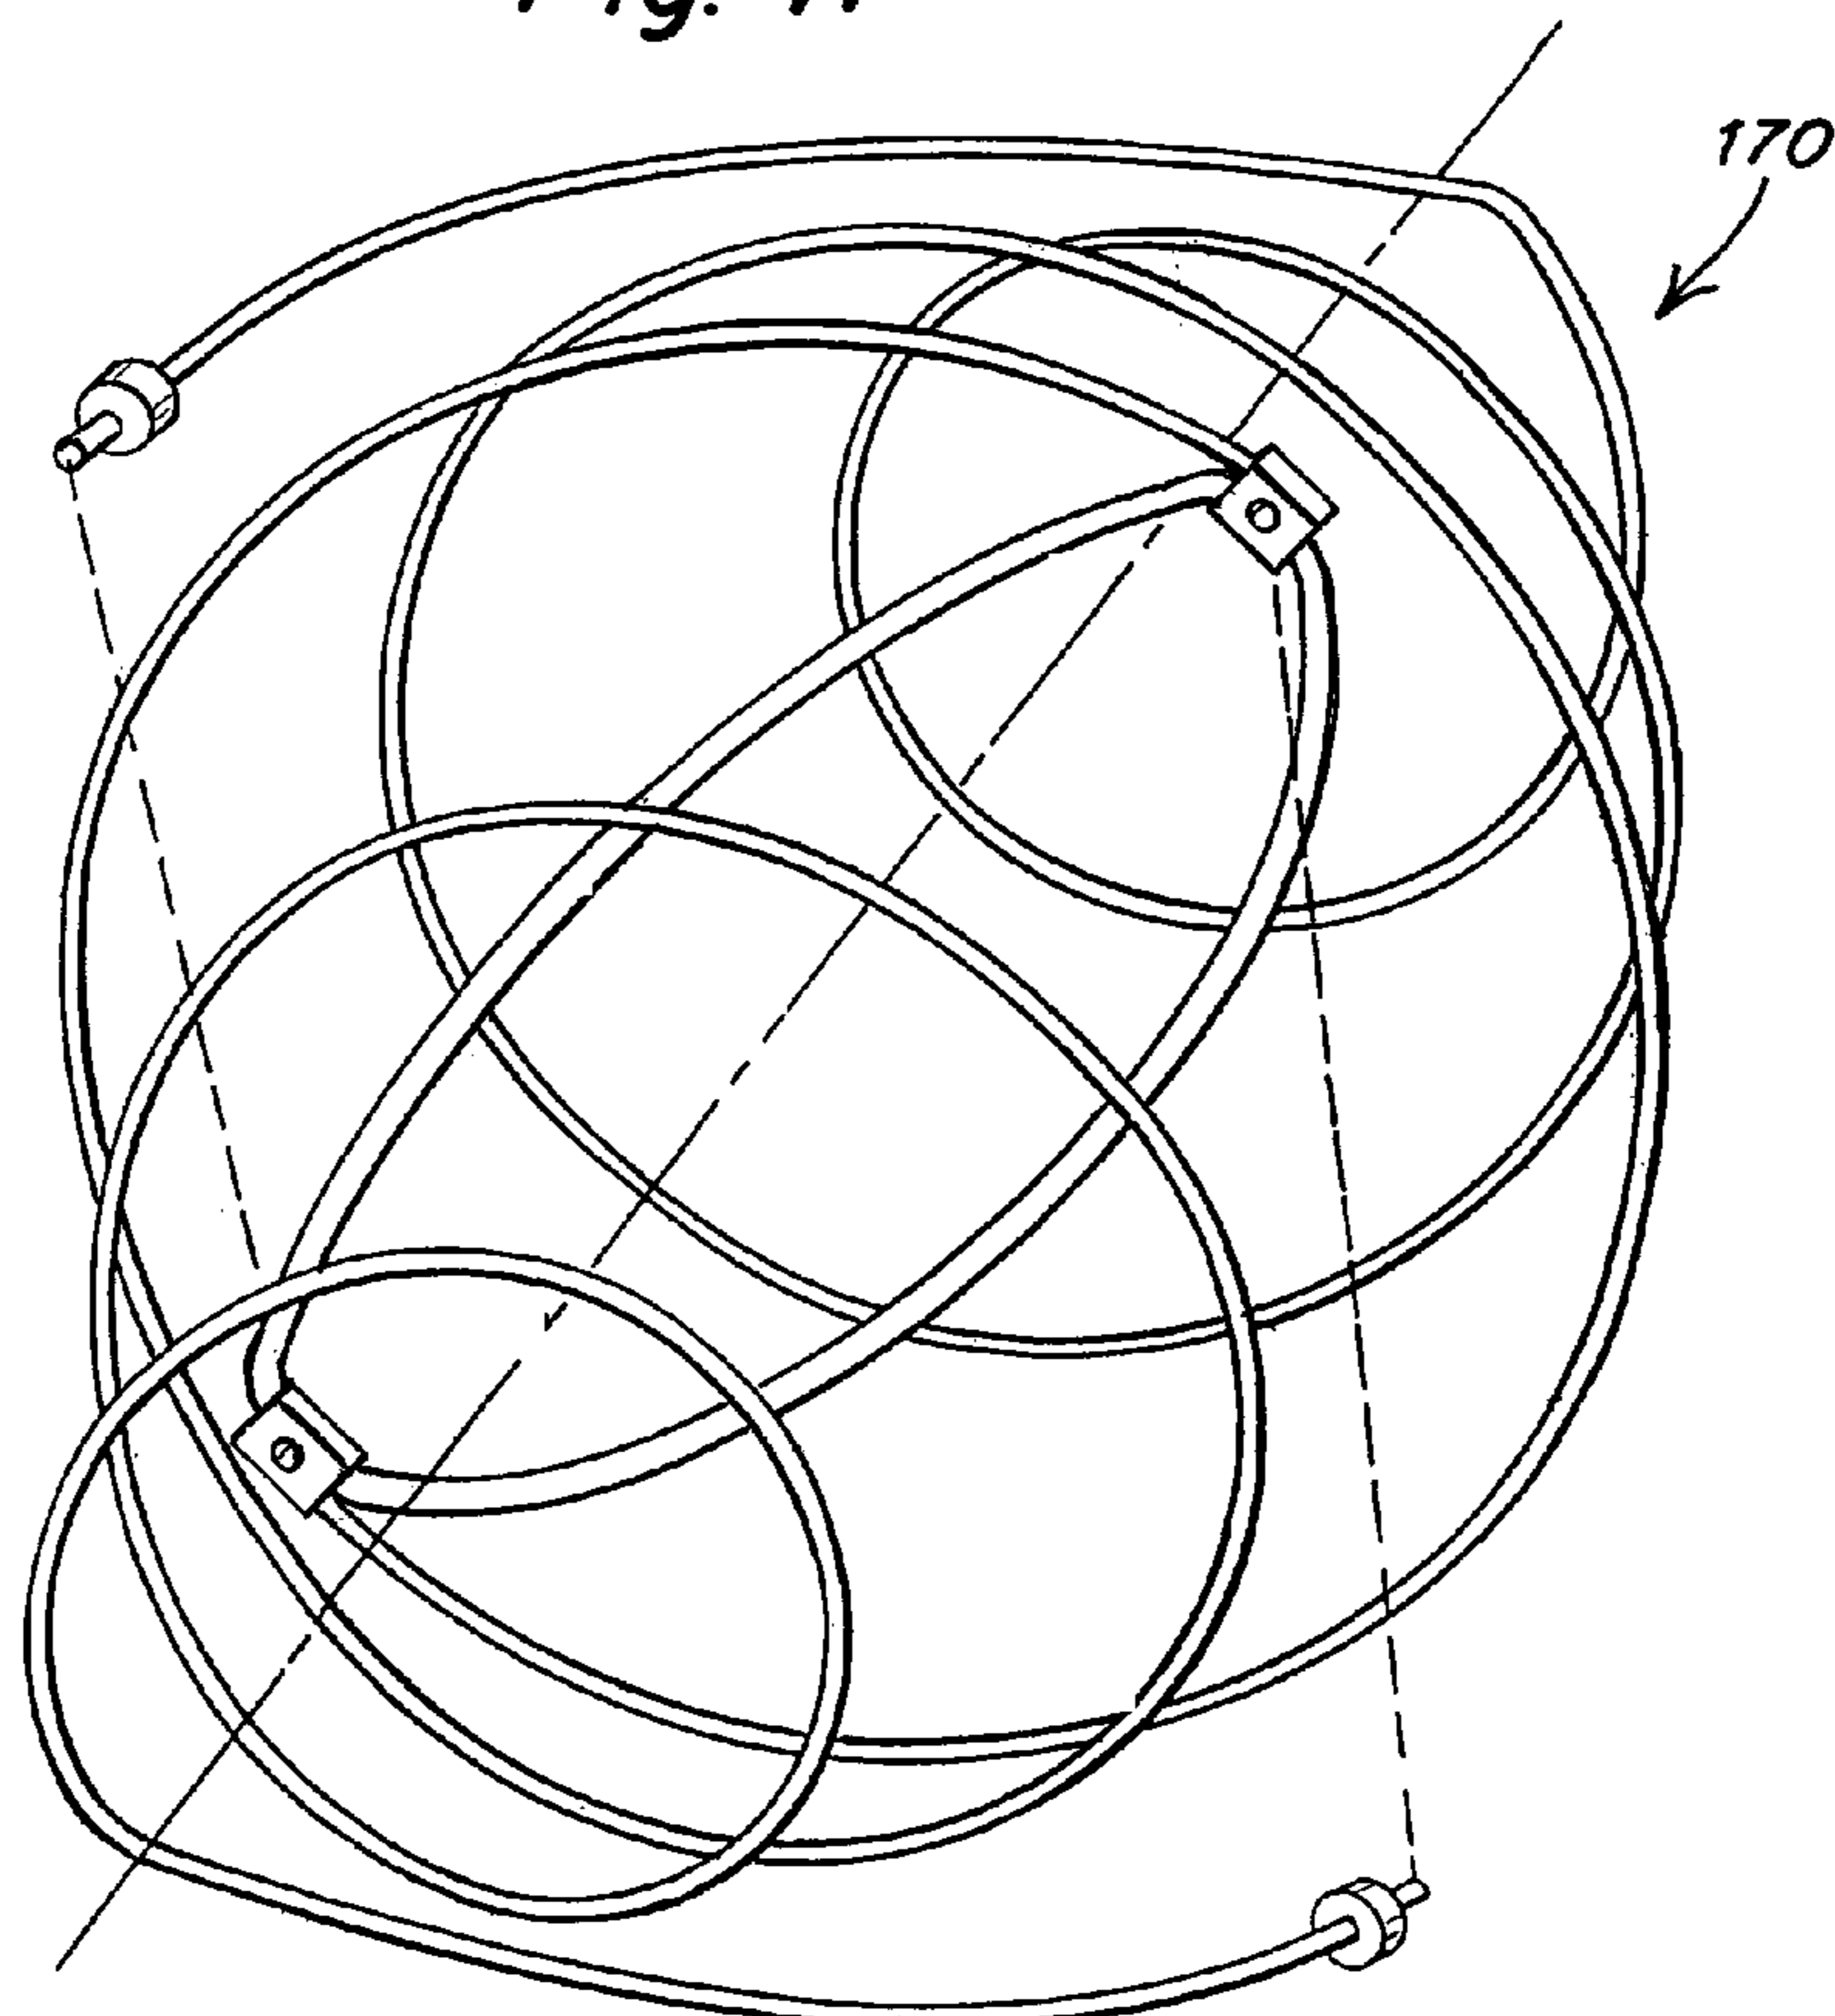


Fig. 18

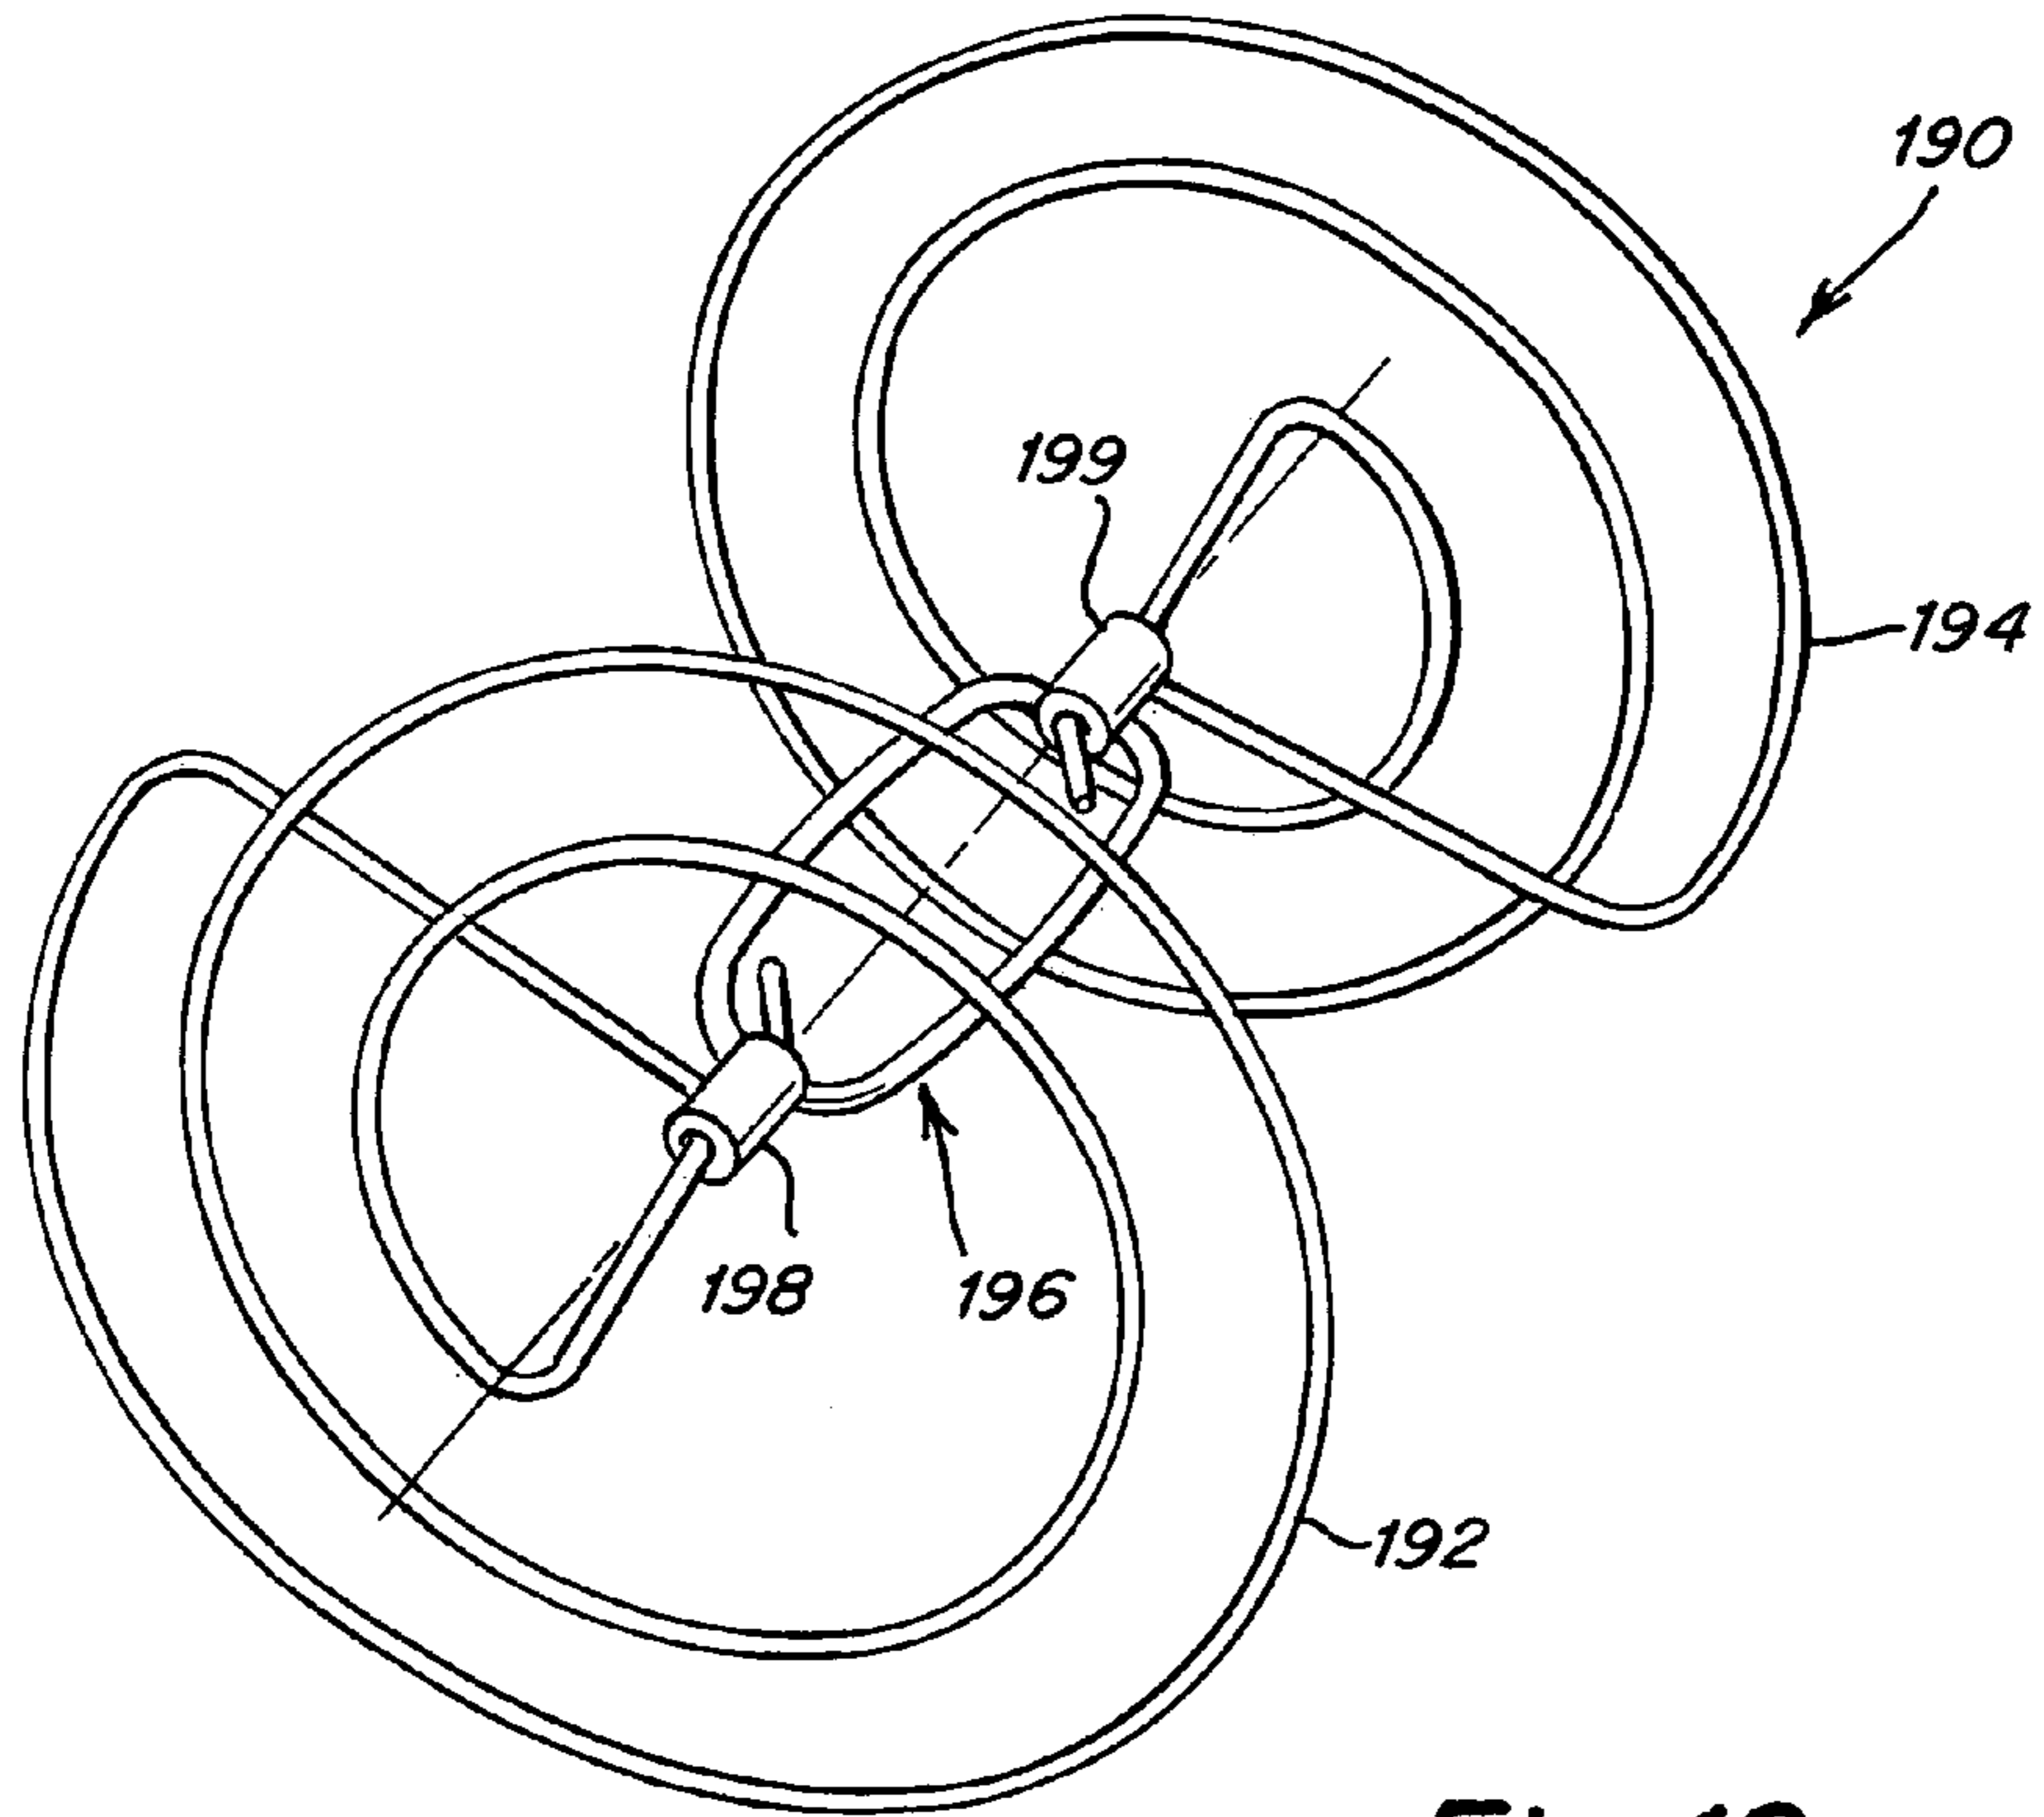


Fig. 19

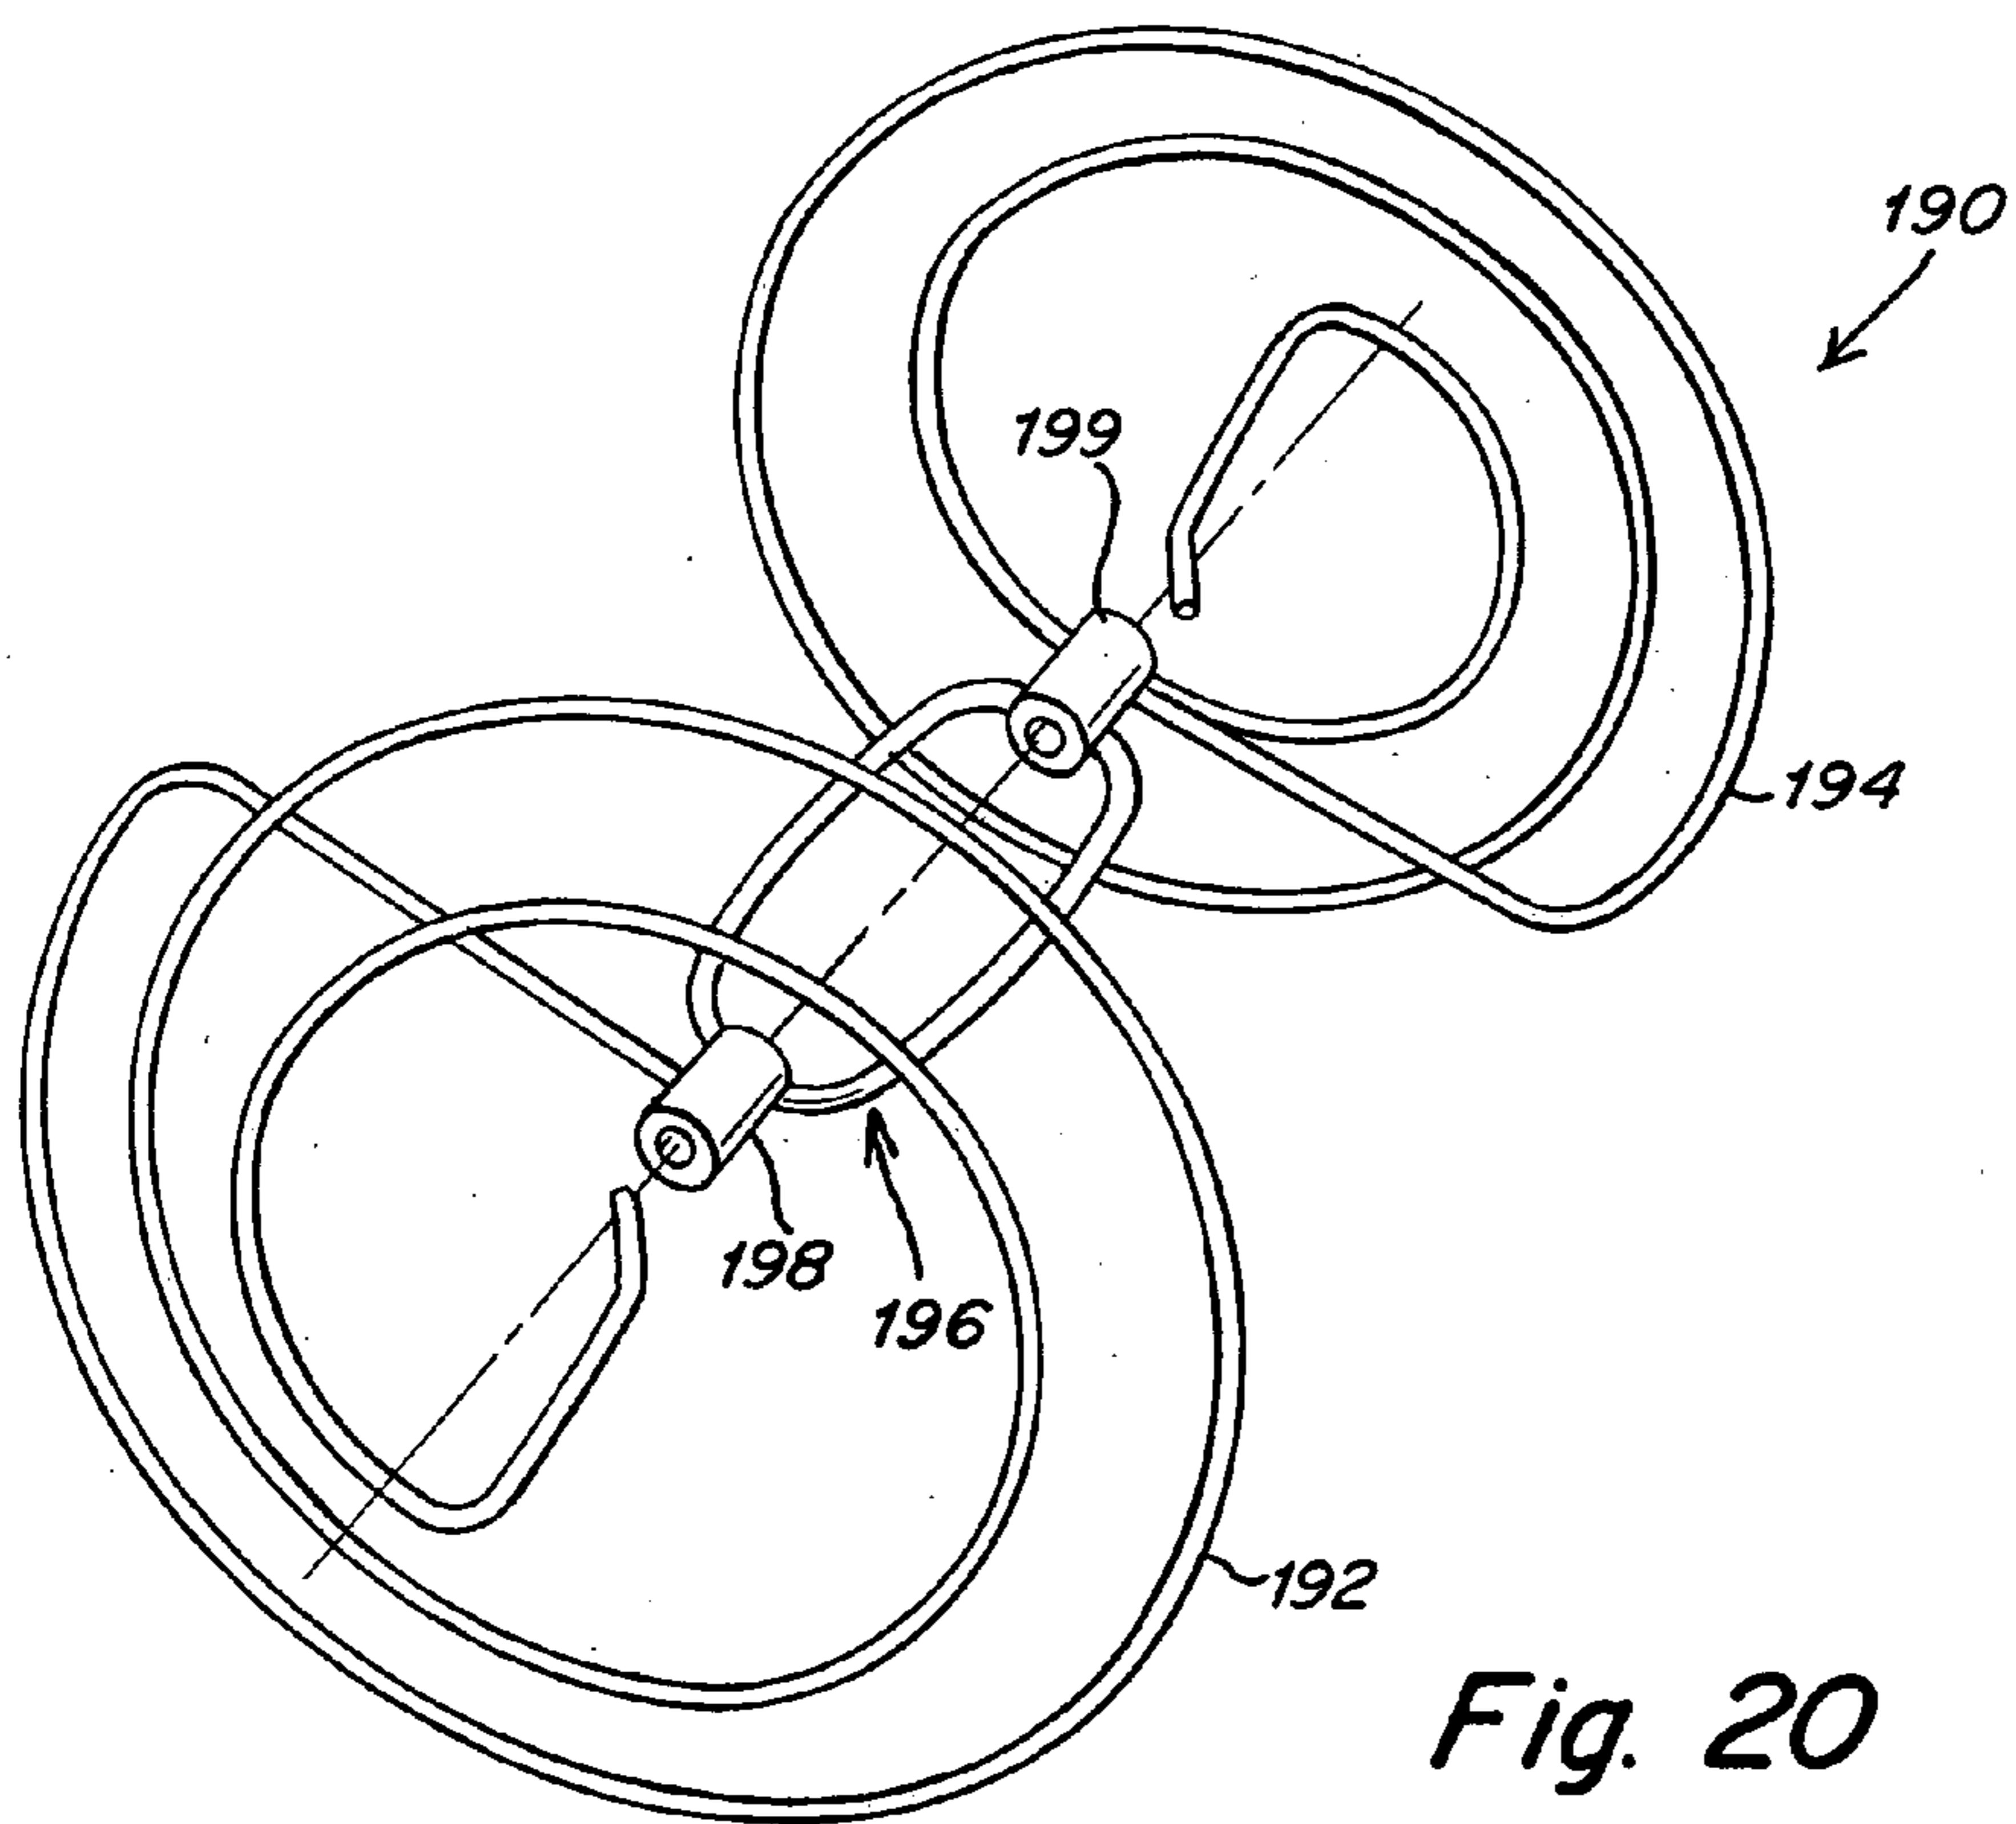


Fig. 20

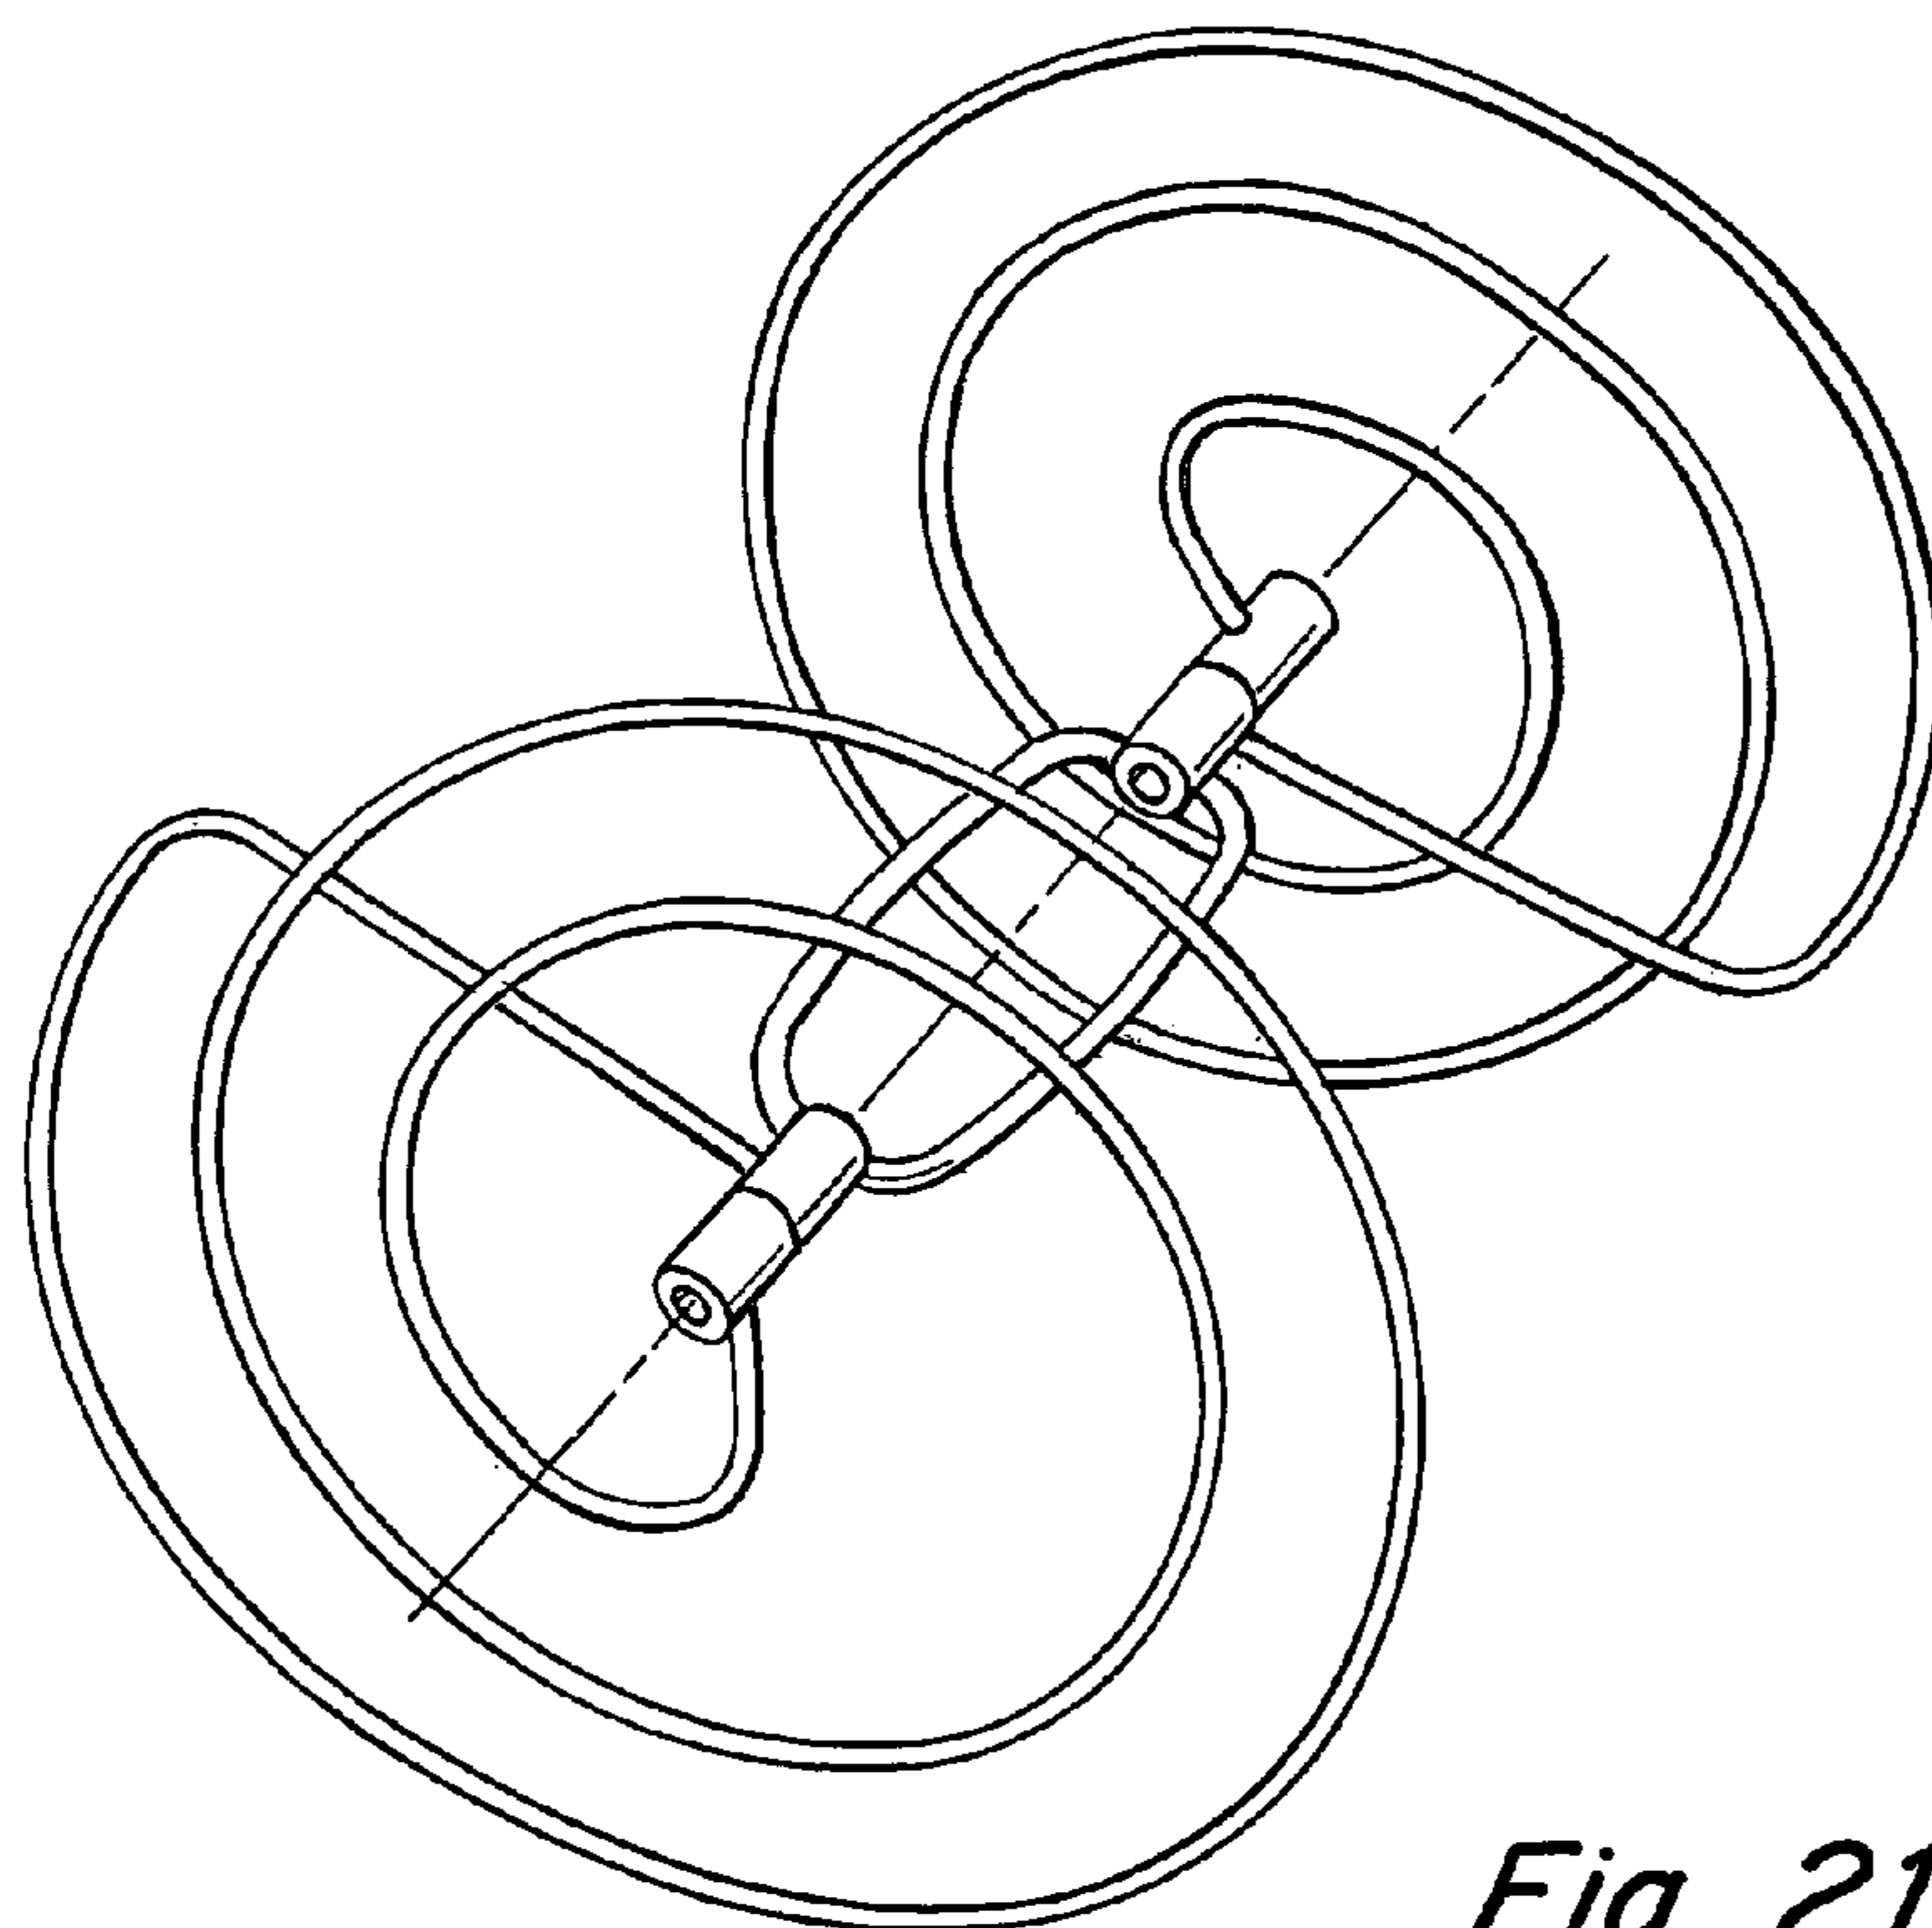


Fig. 21

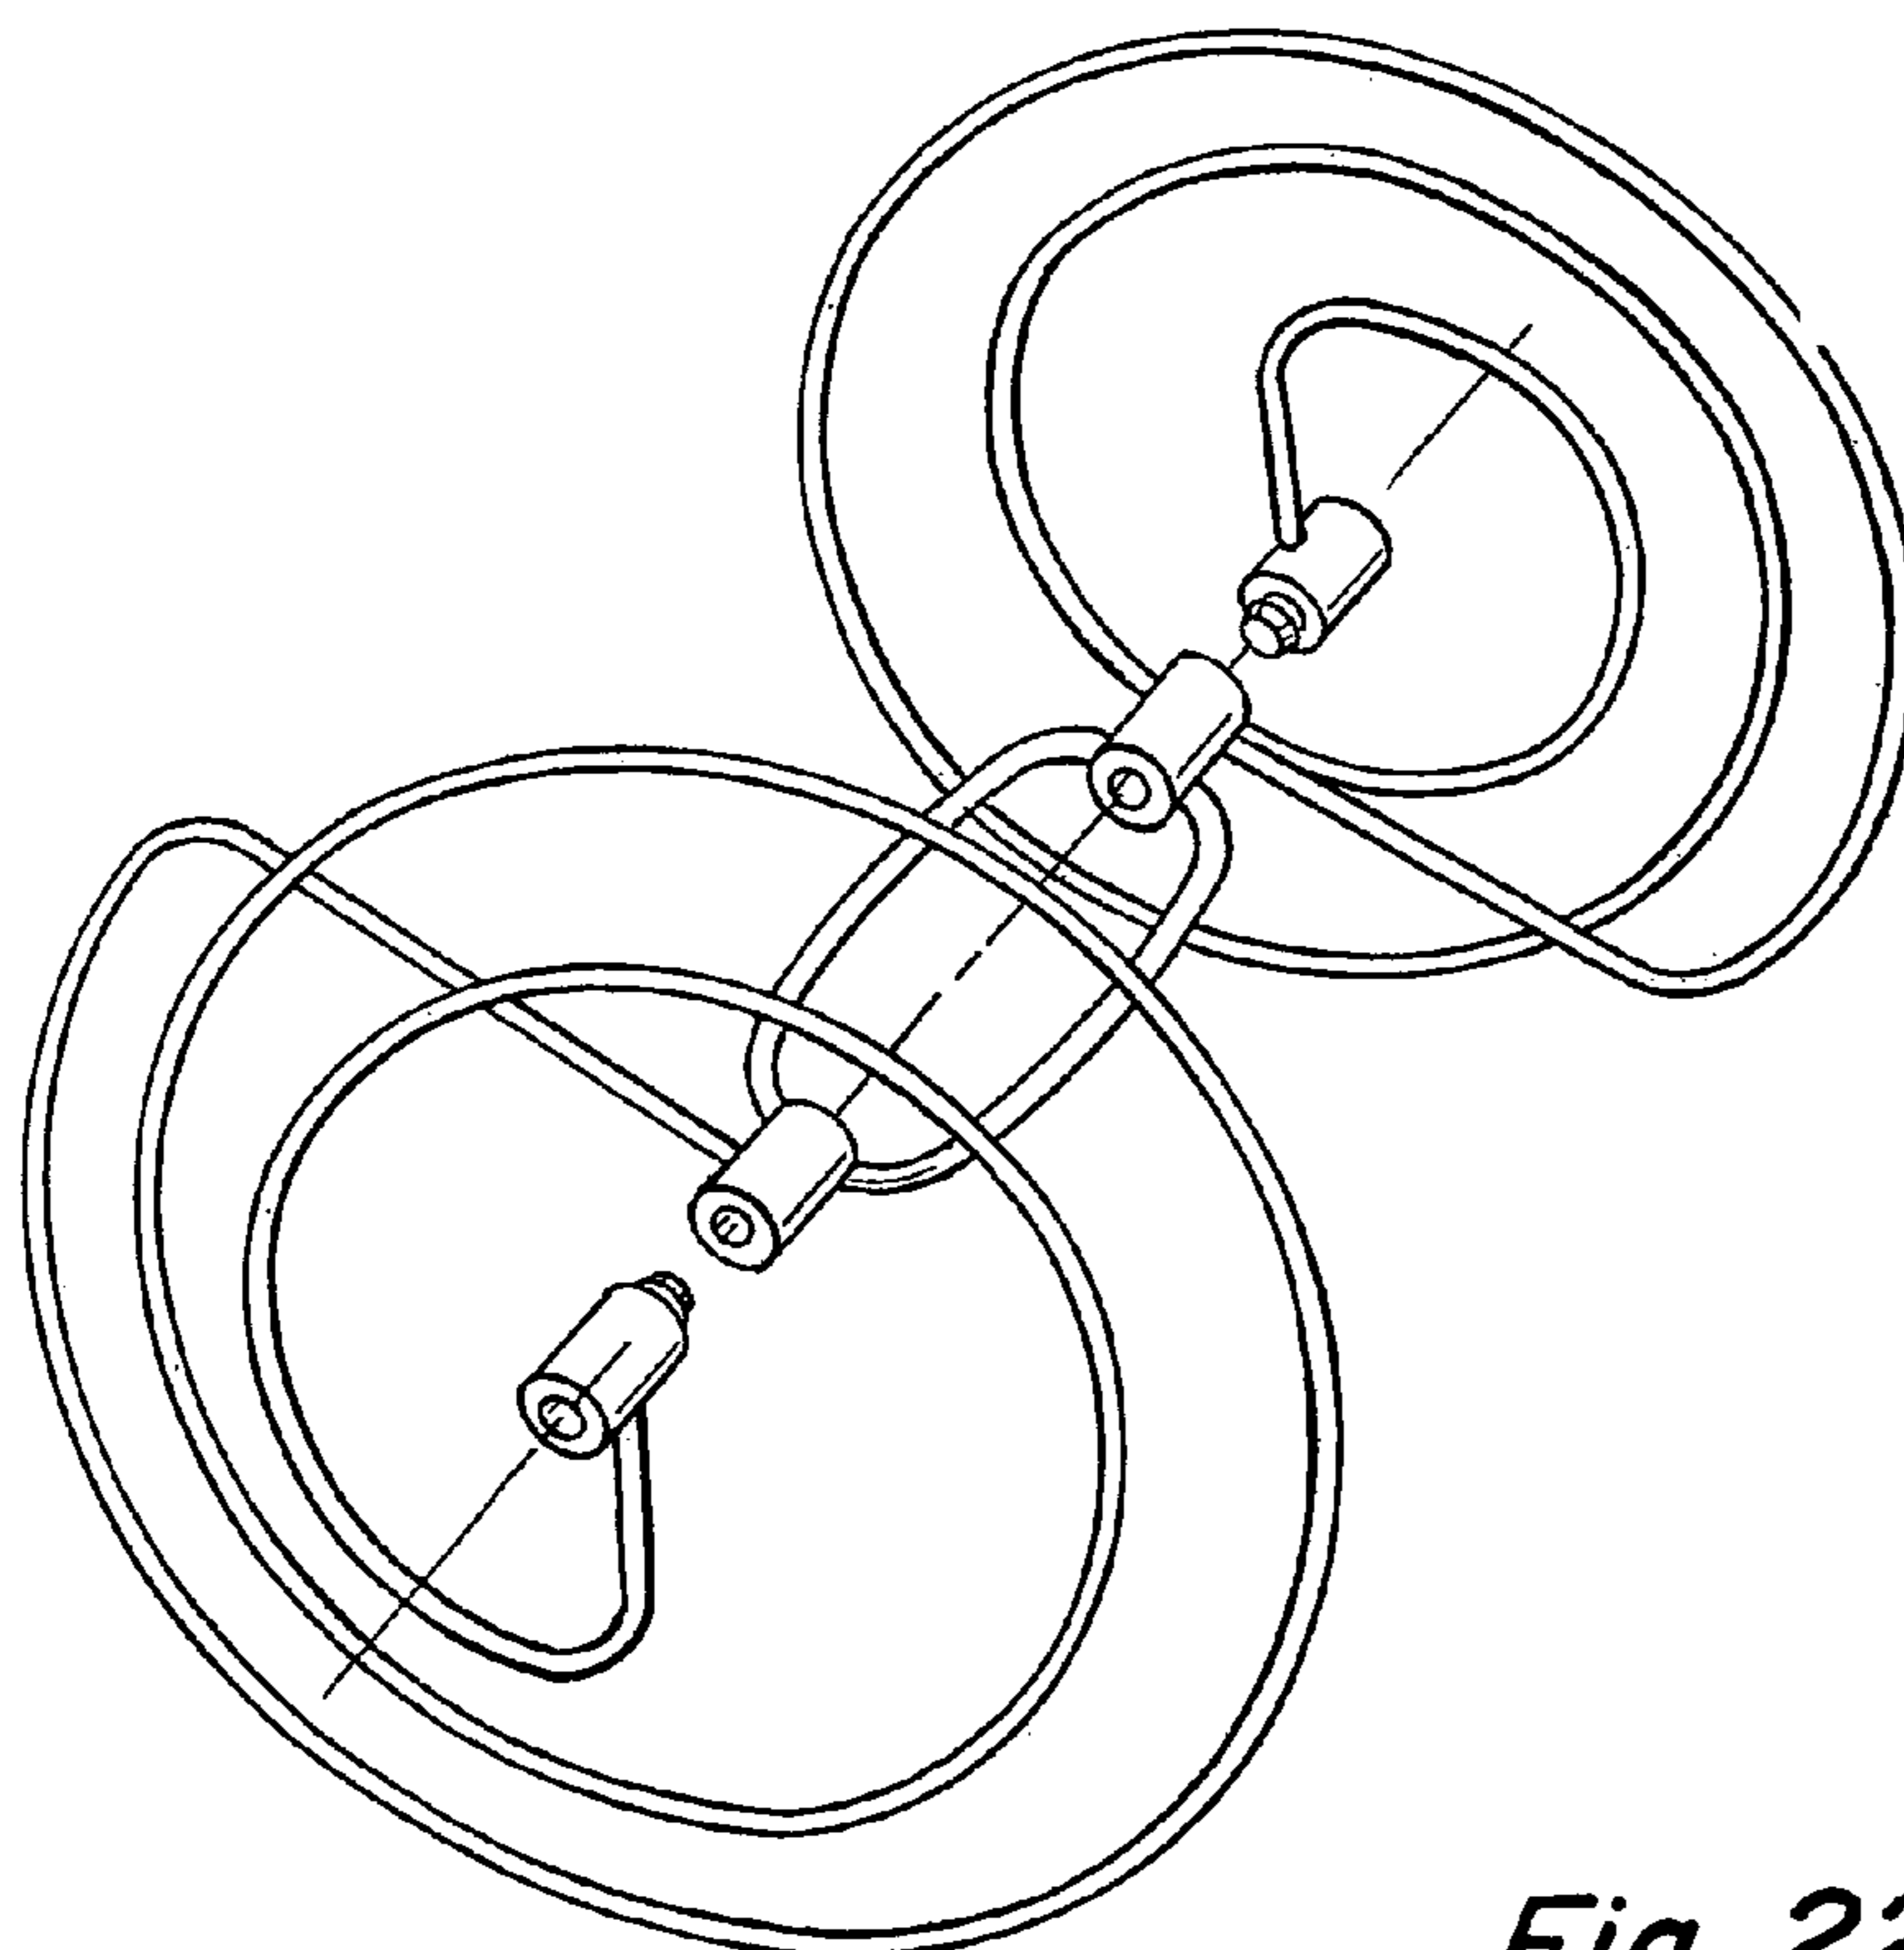


Fig. 22

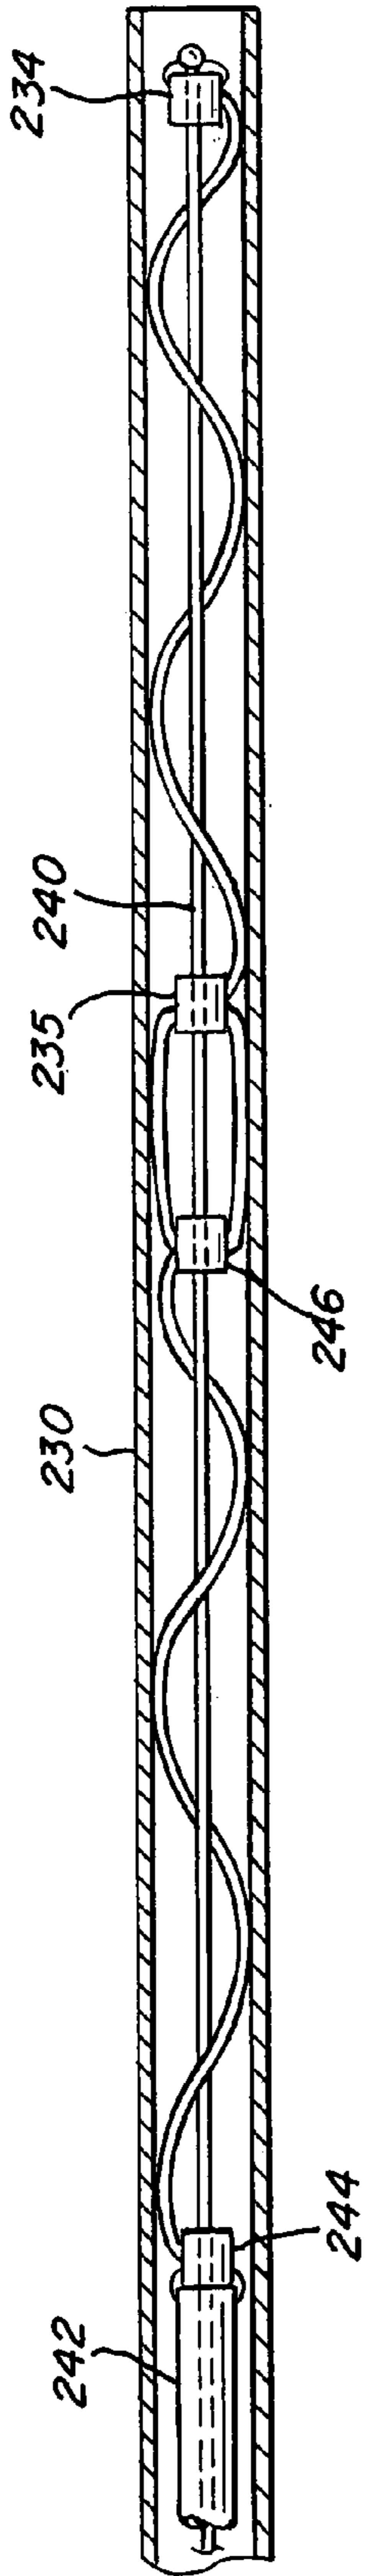


Fig. 23

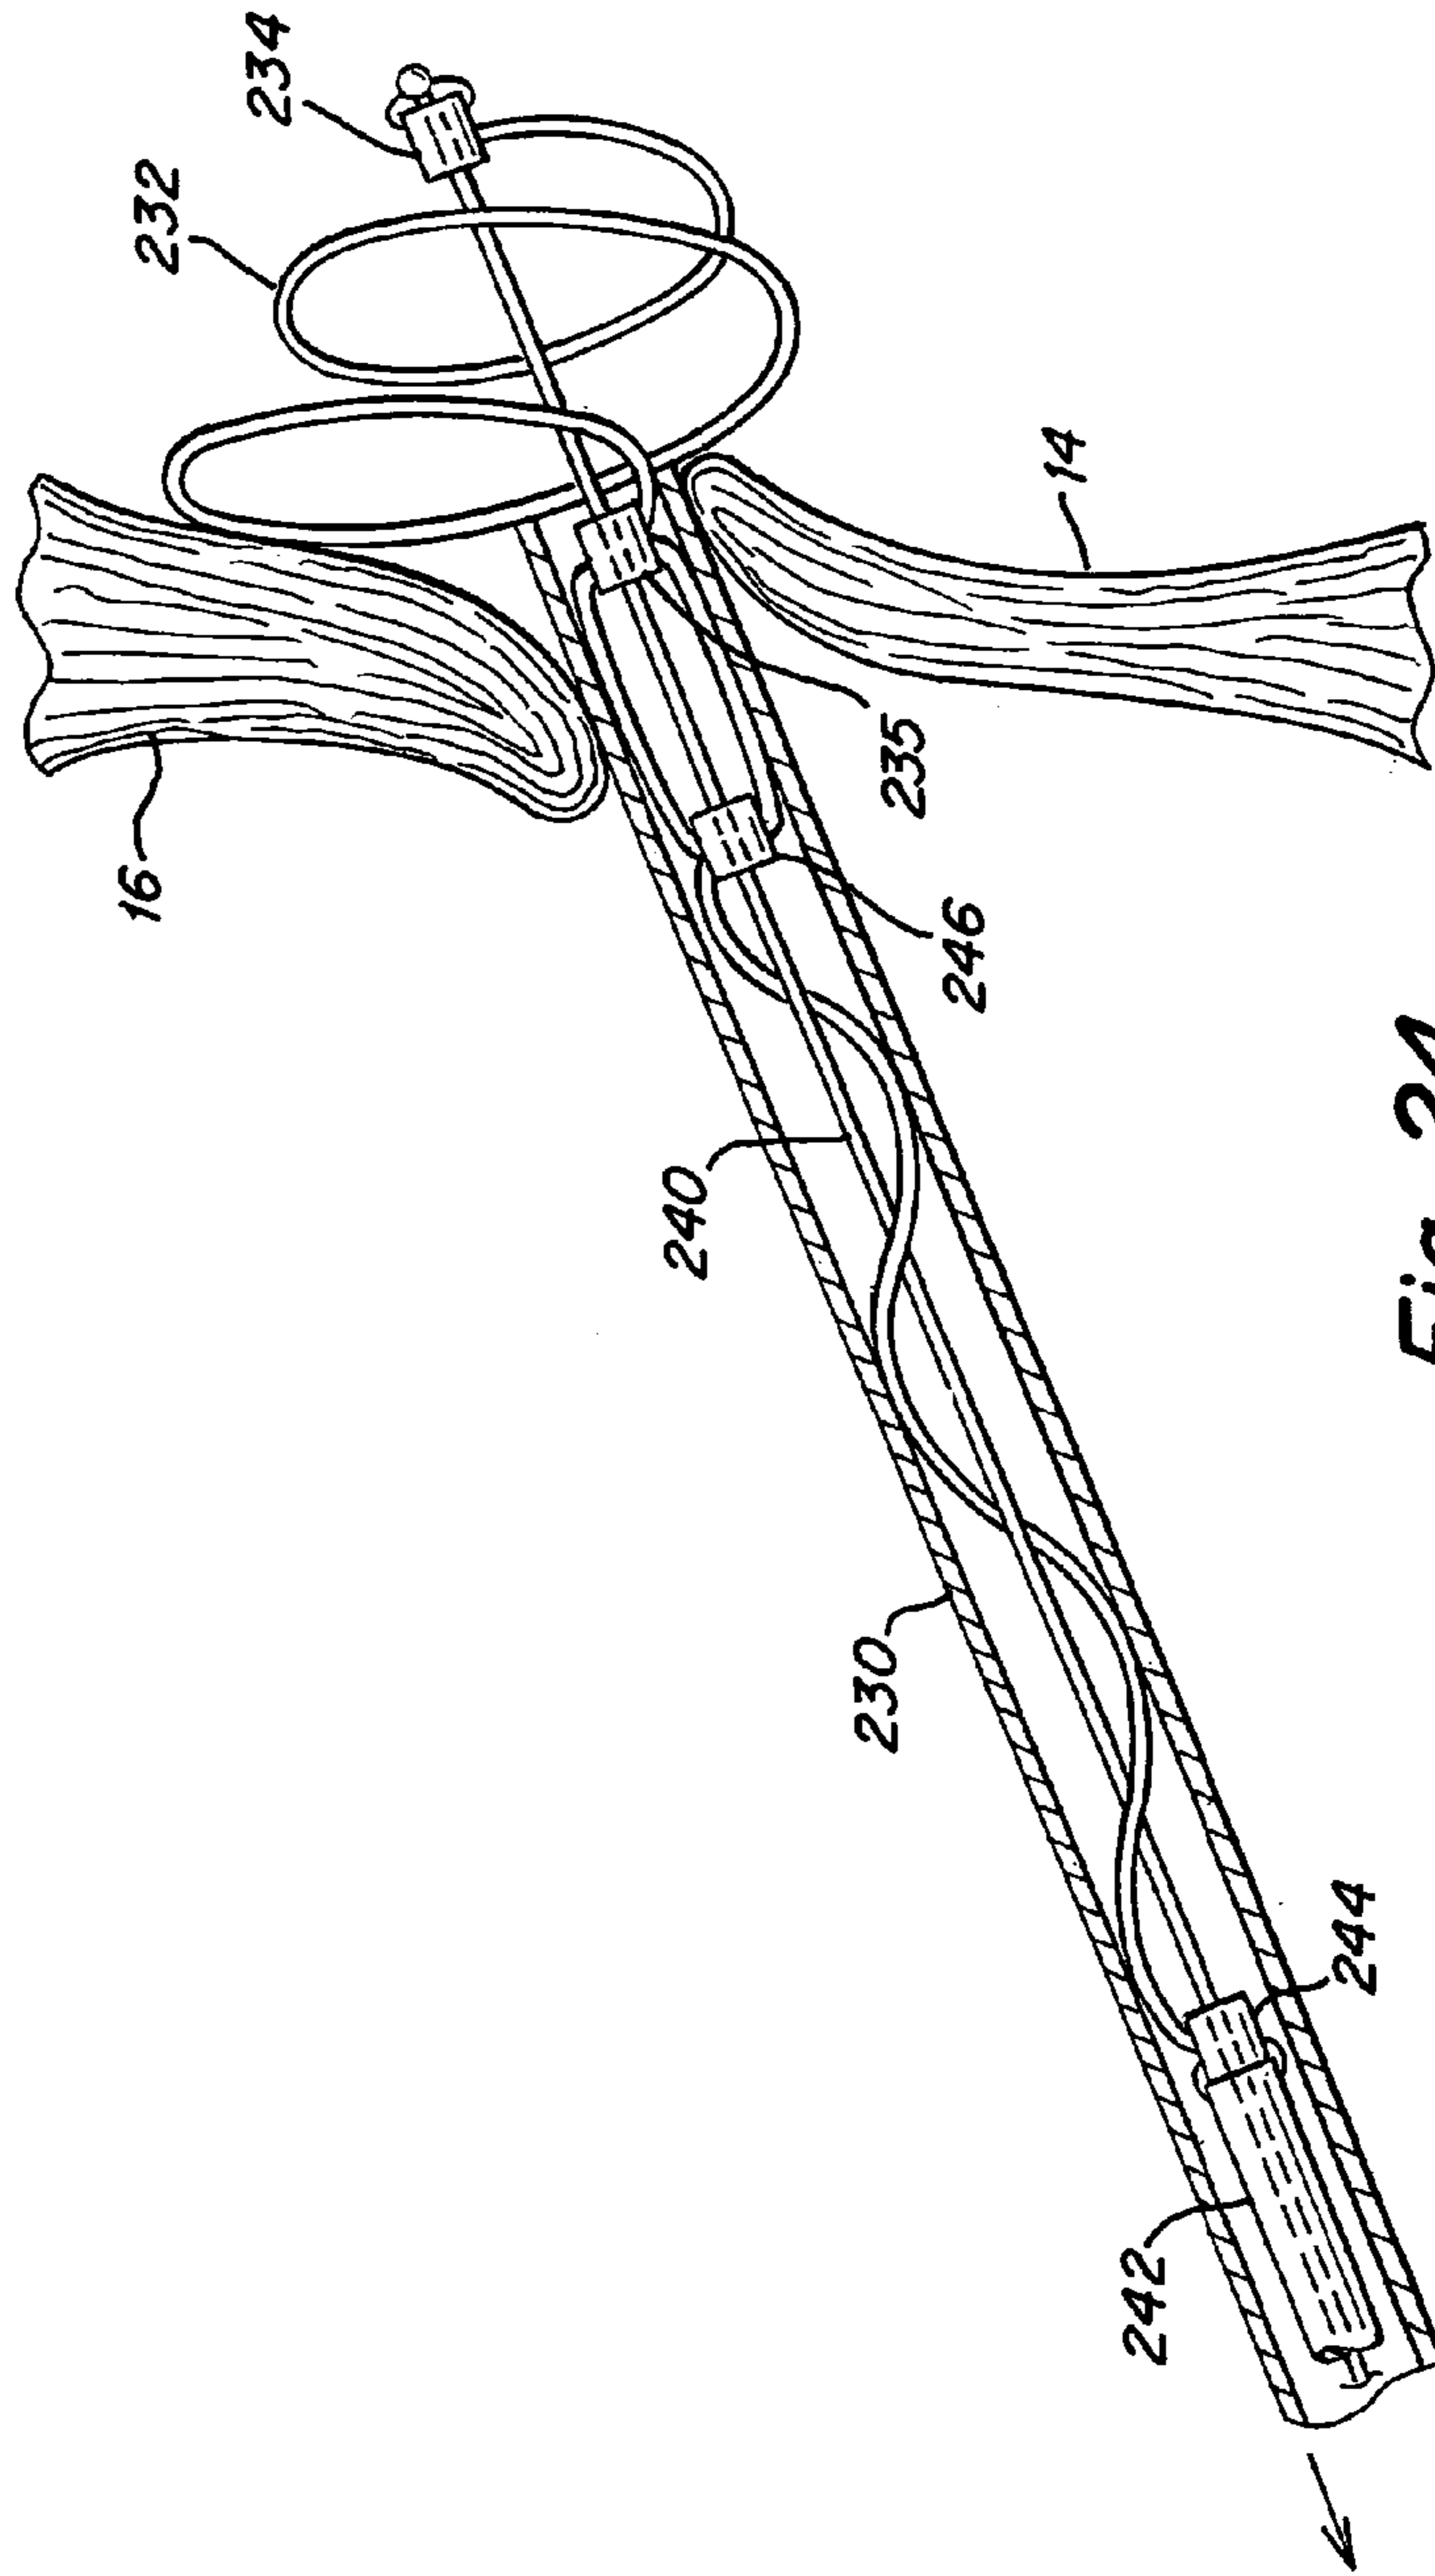


Fig. 24

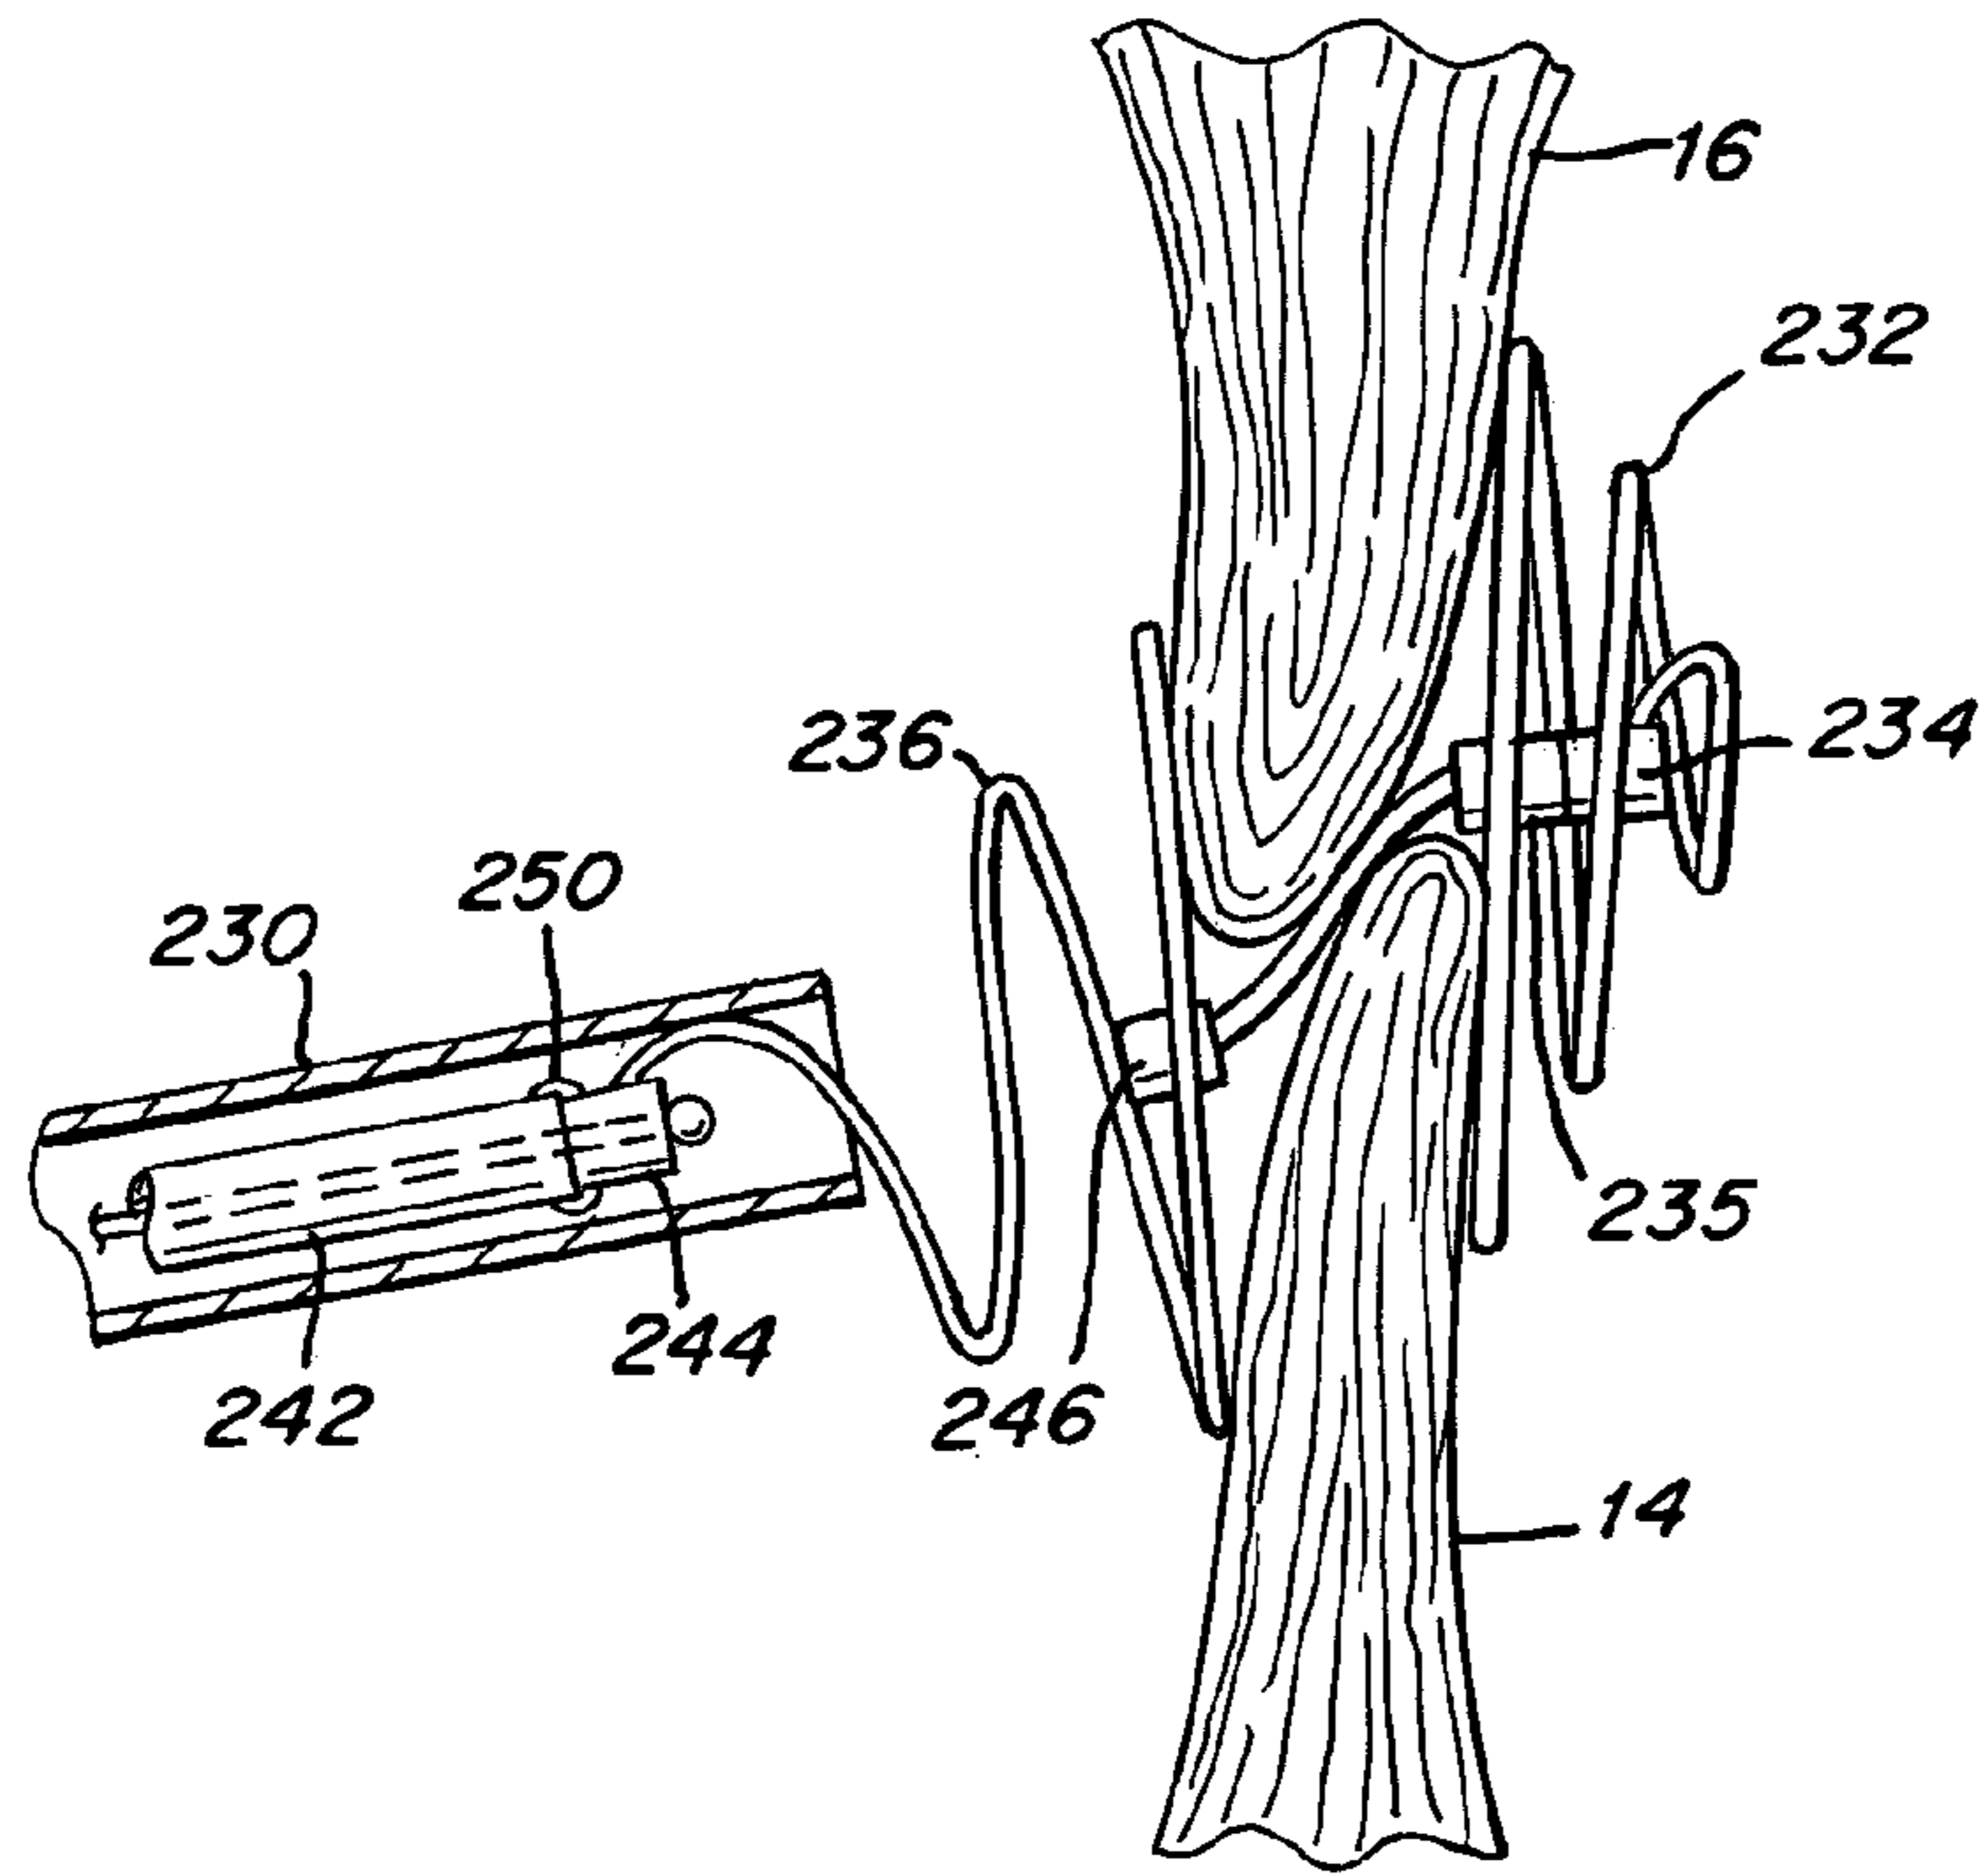


Fig. 25

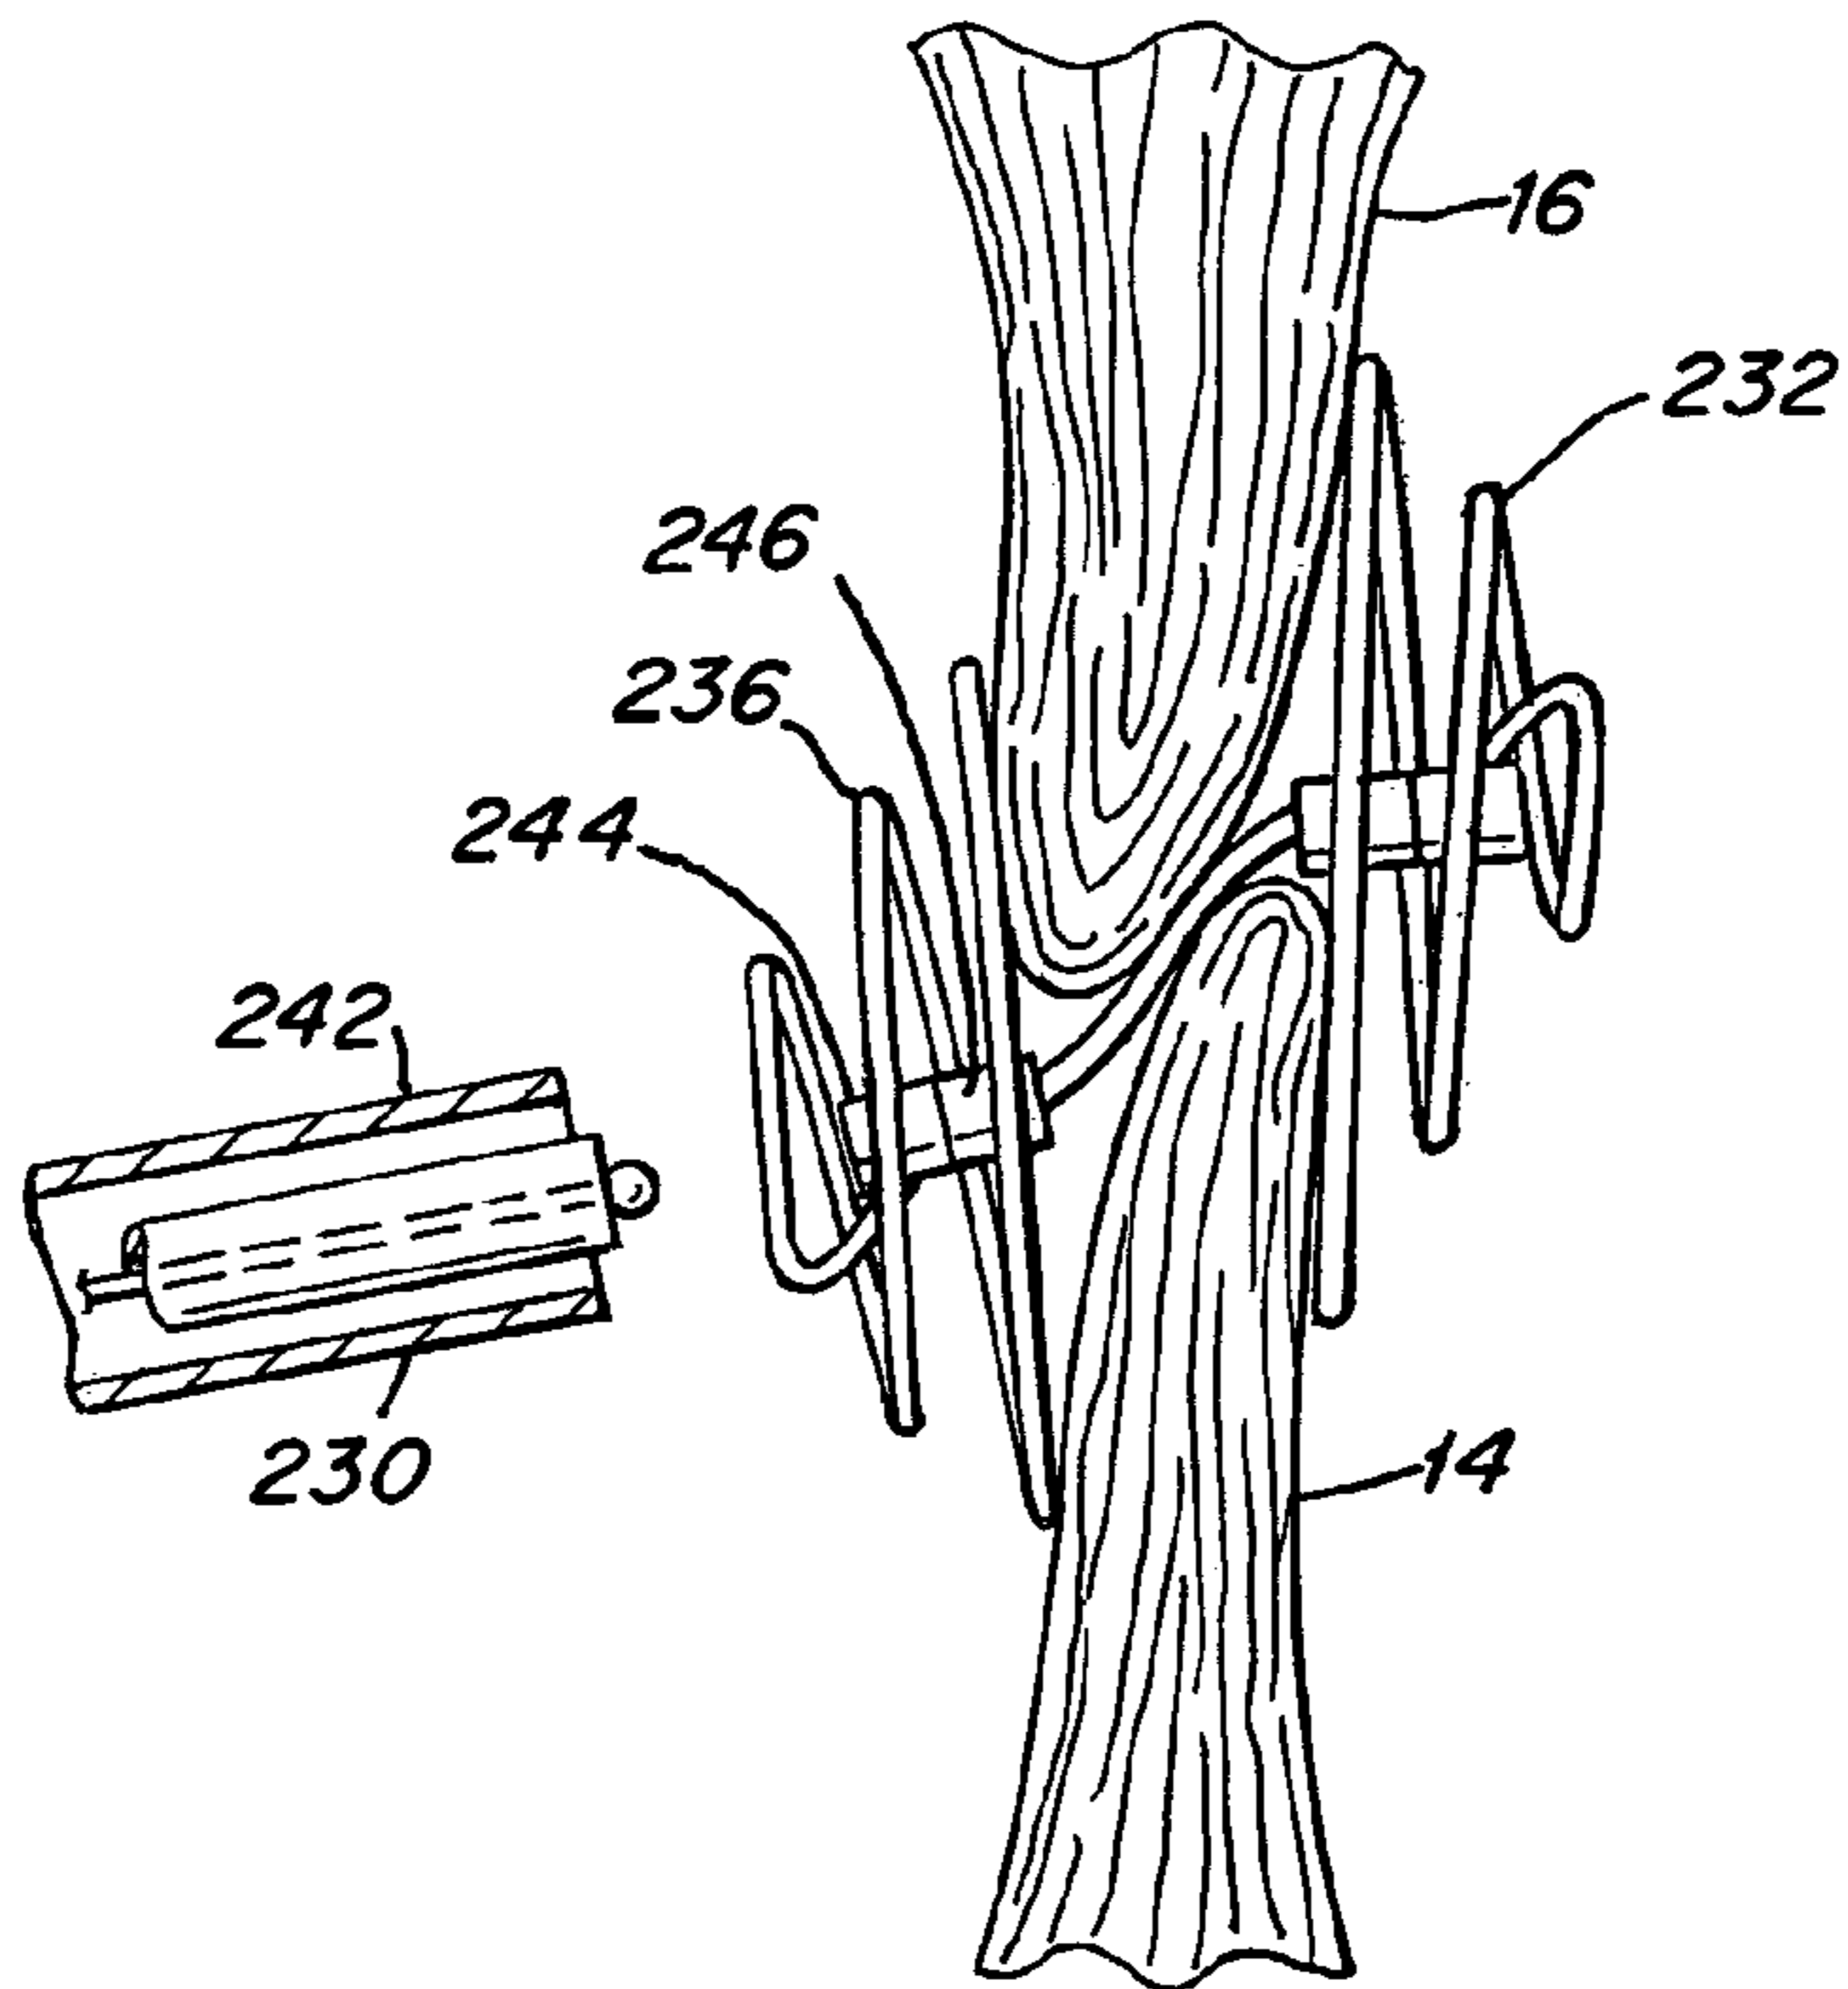


Fig. 26

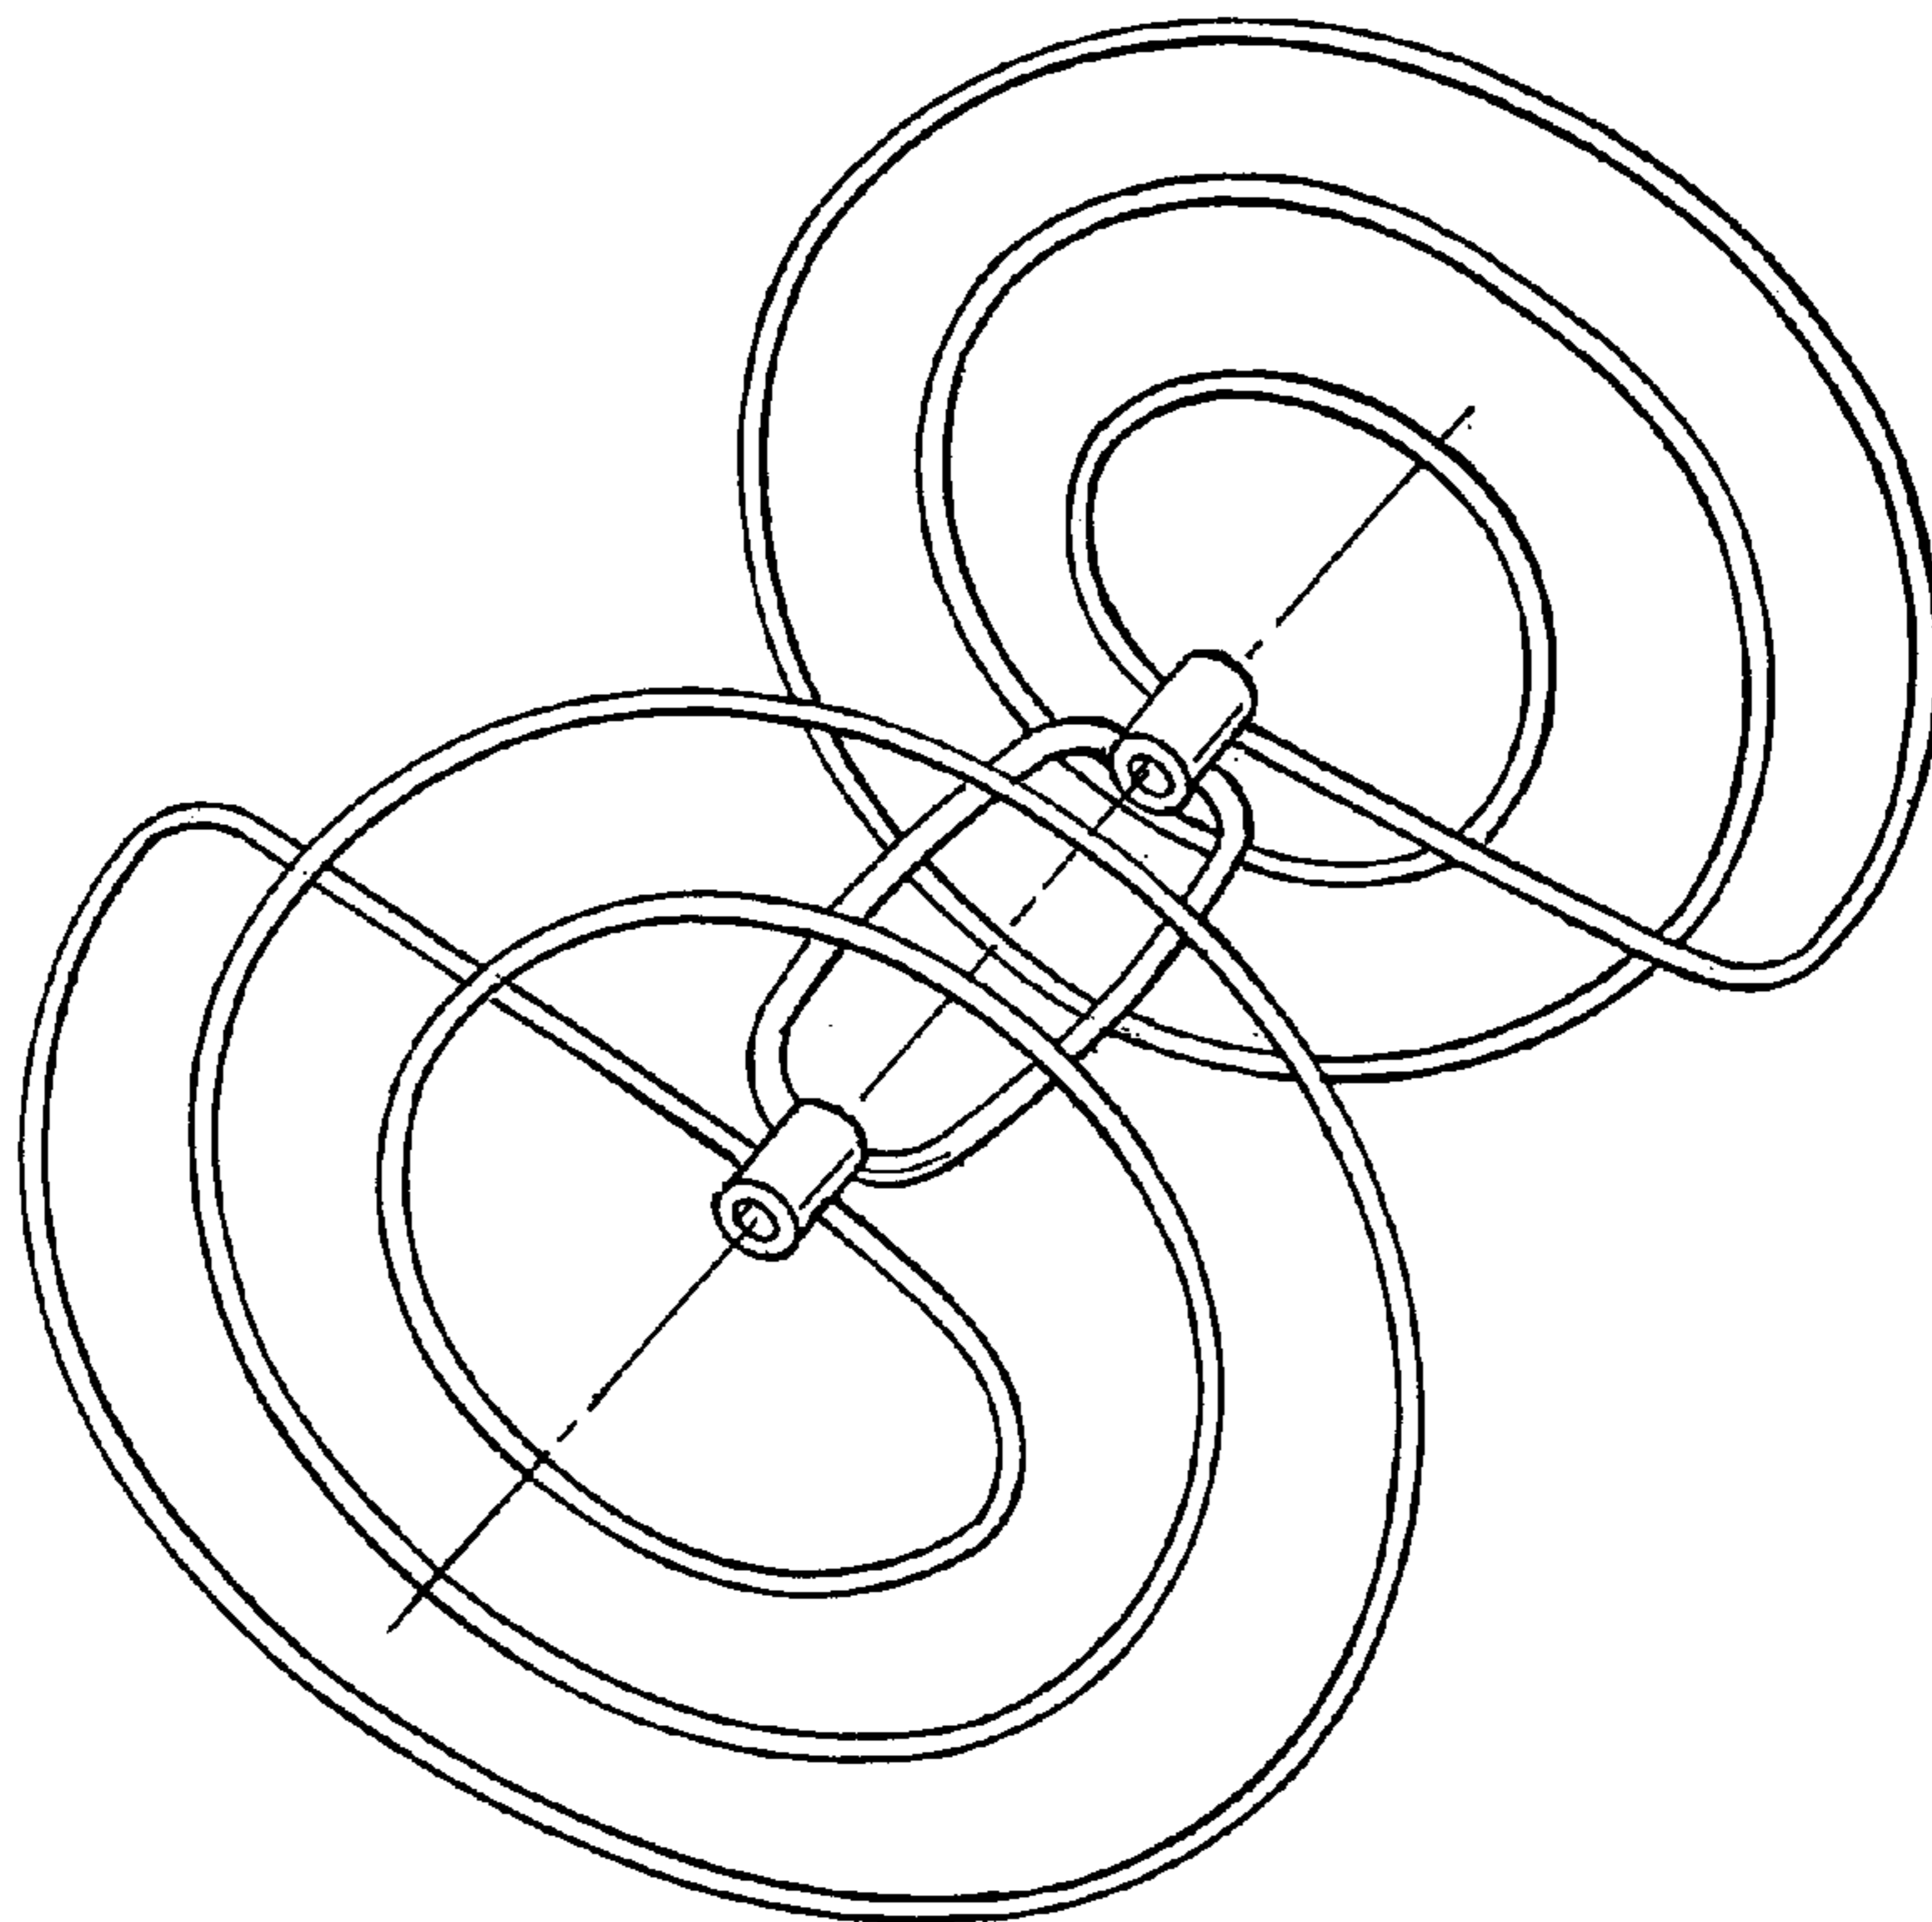


Fig. 27

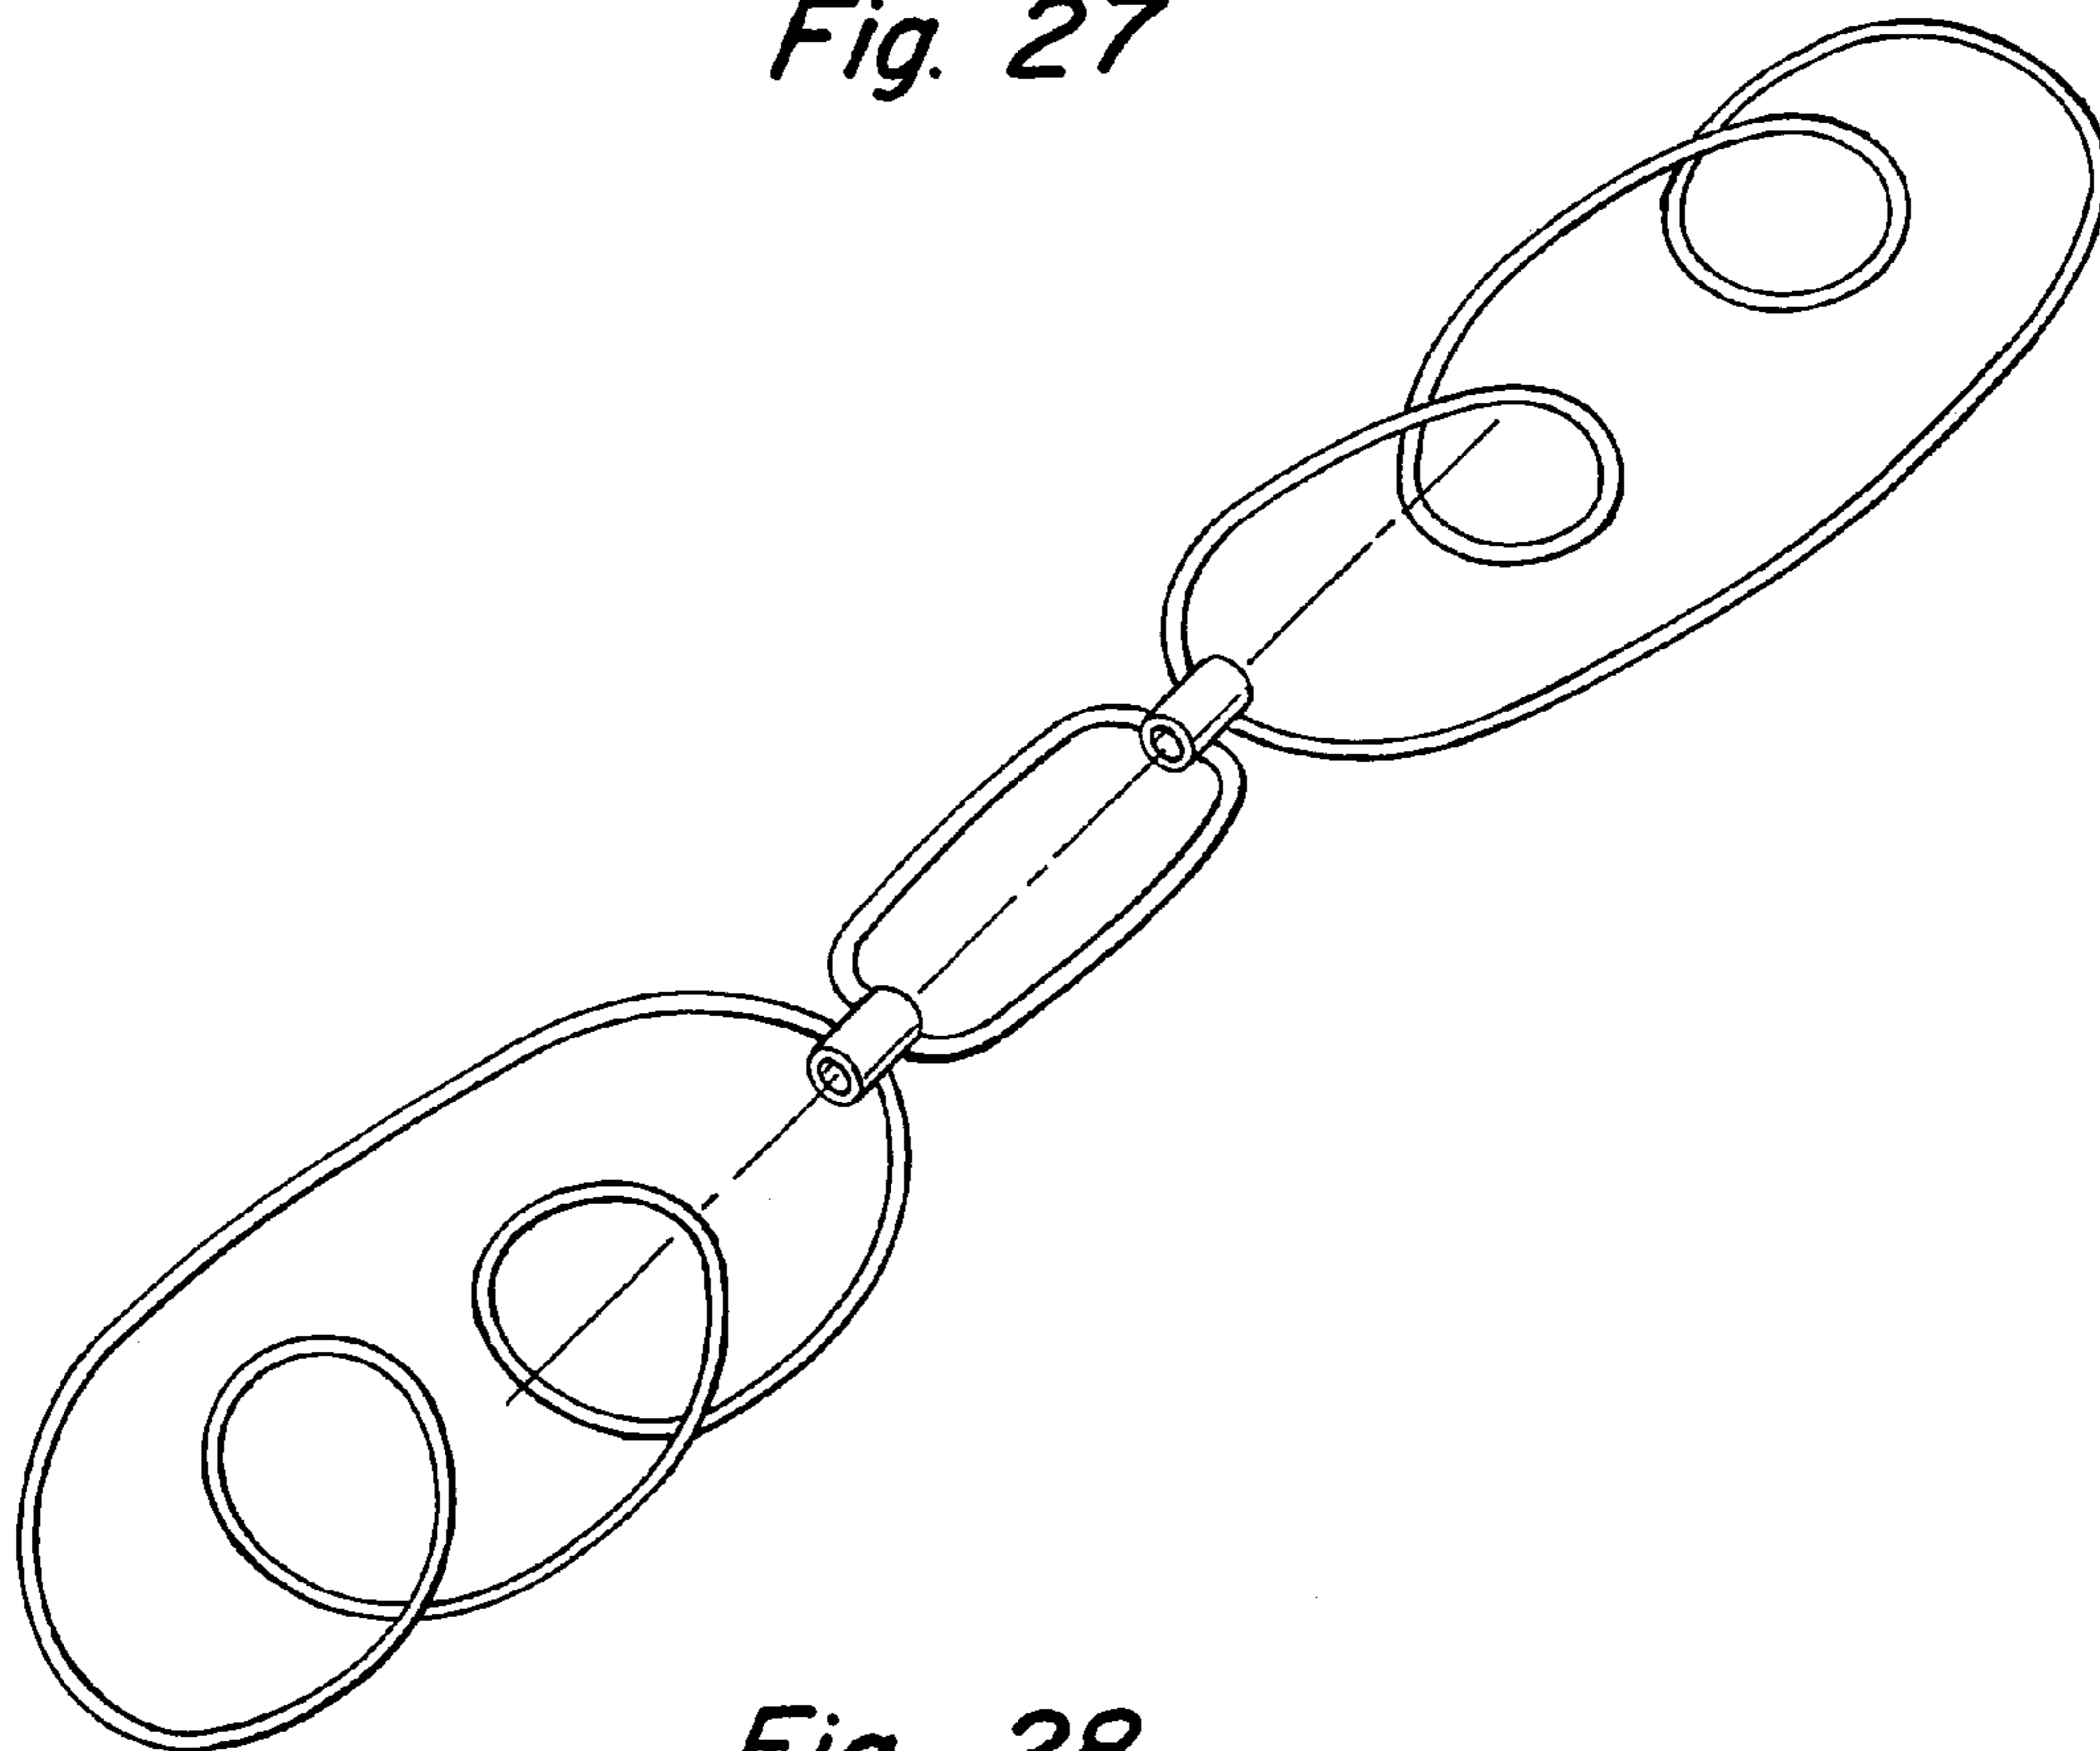


Fig. 28

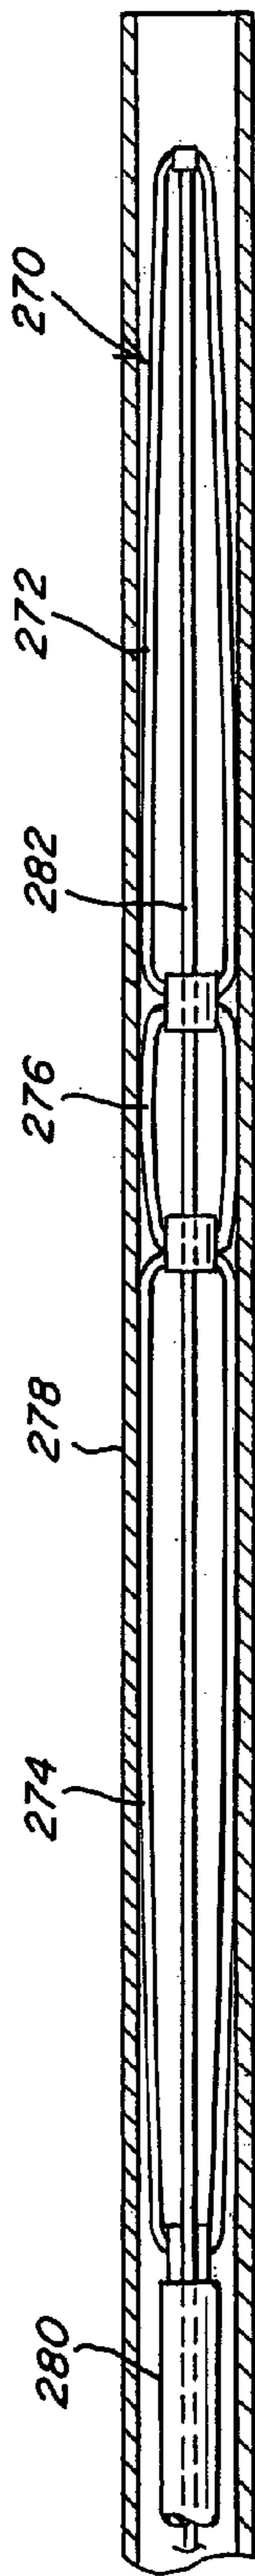


Fig. 29

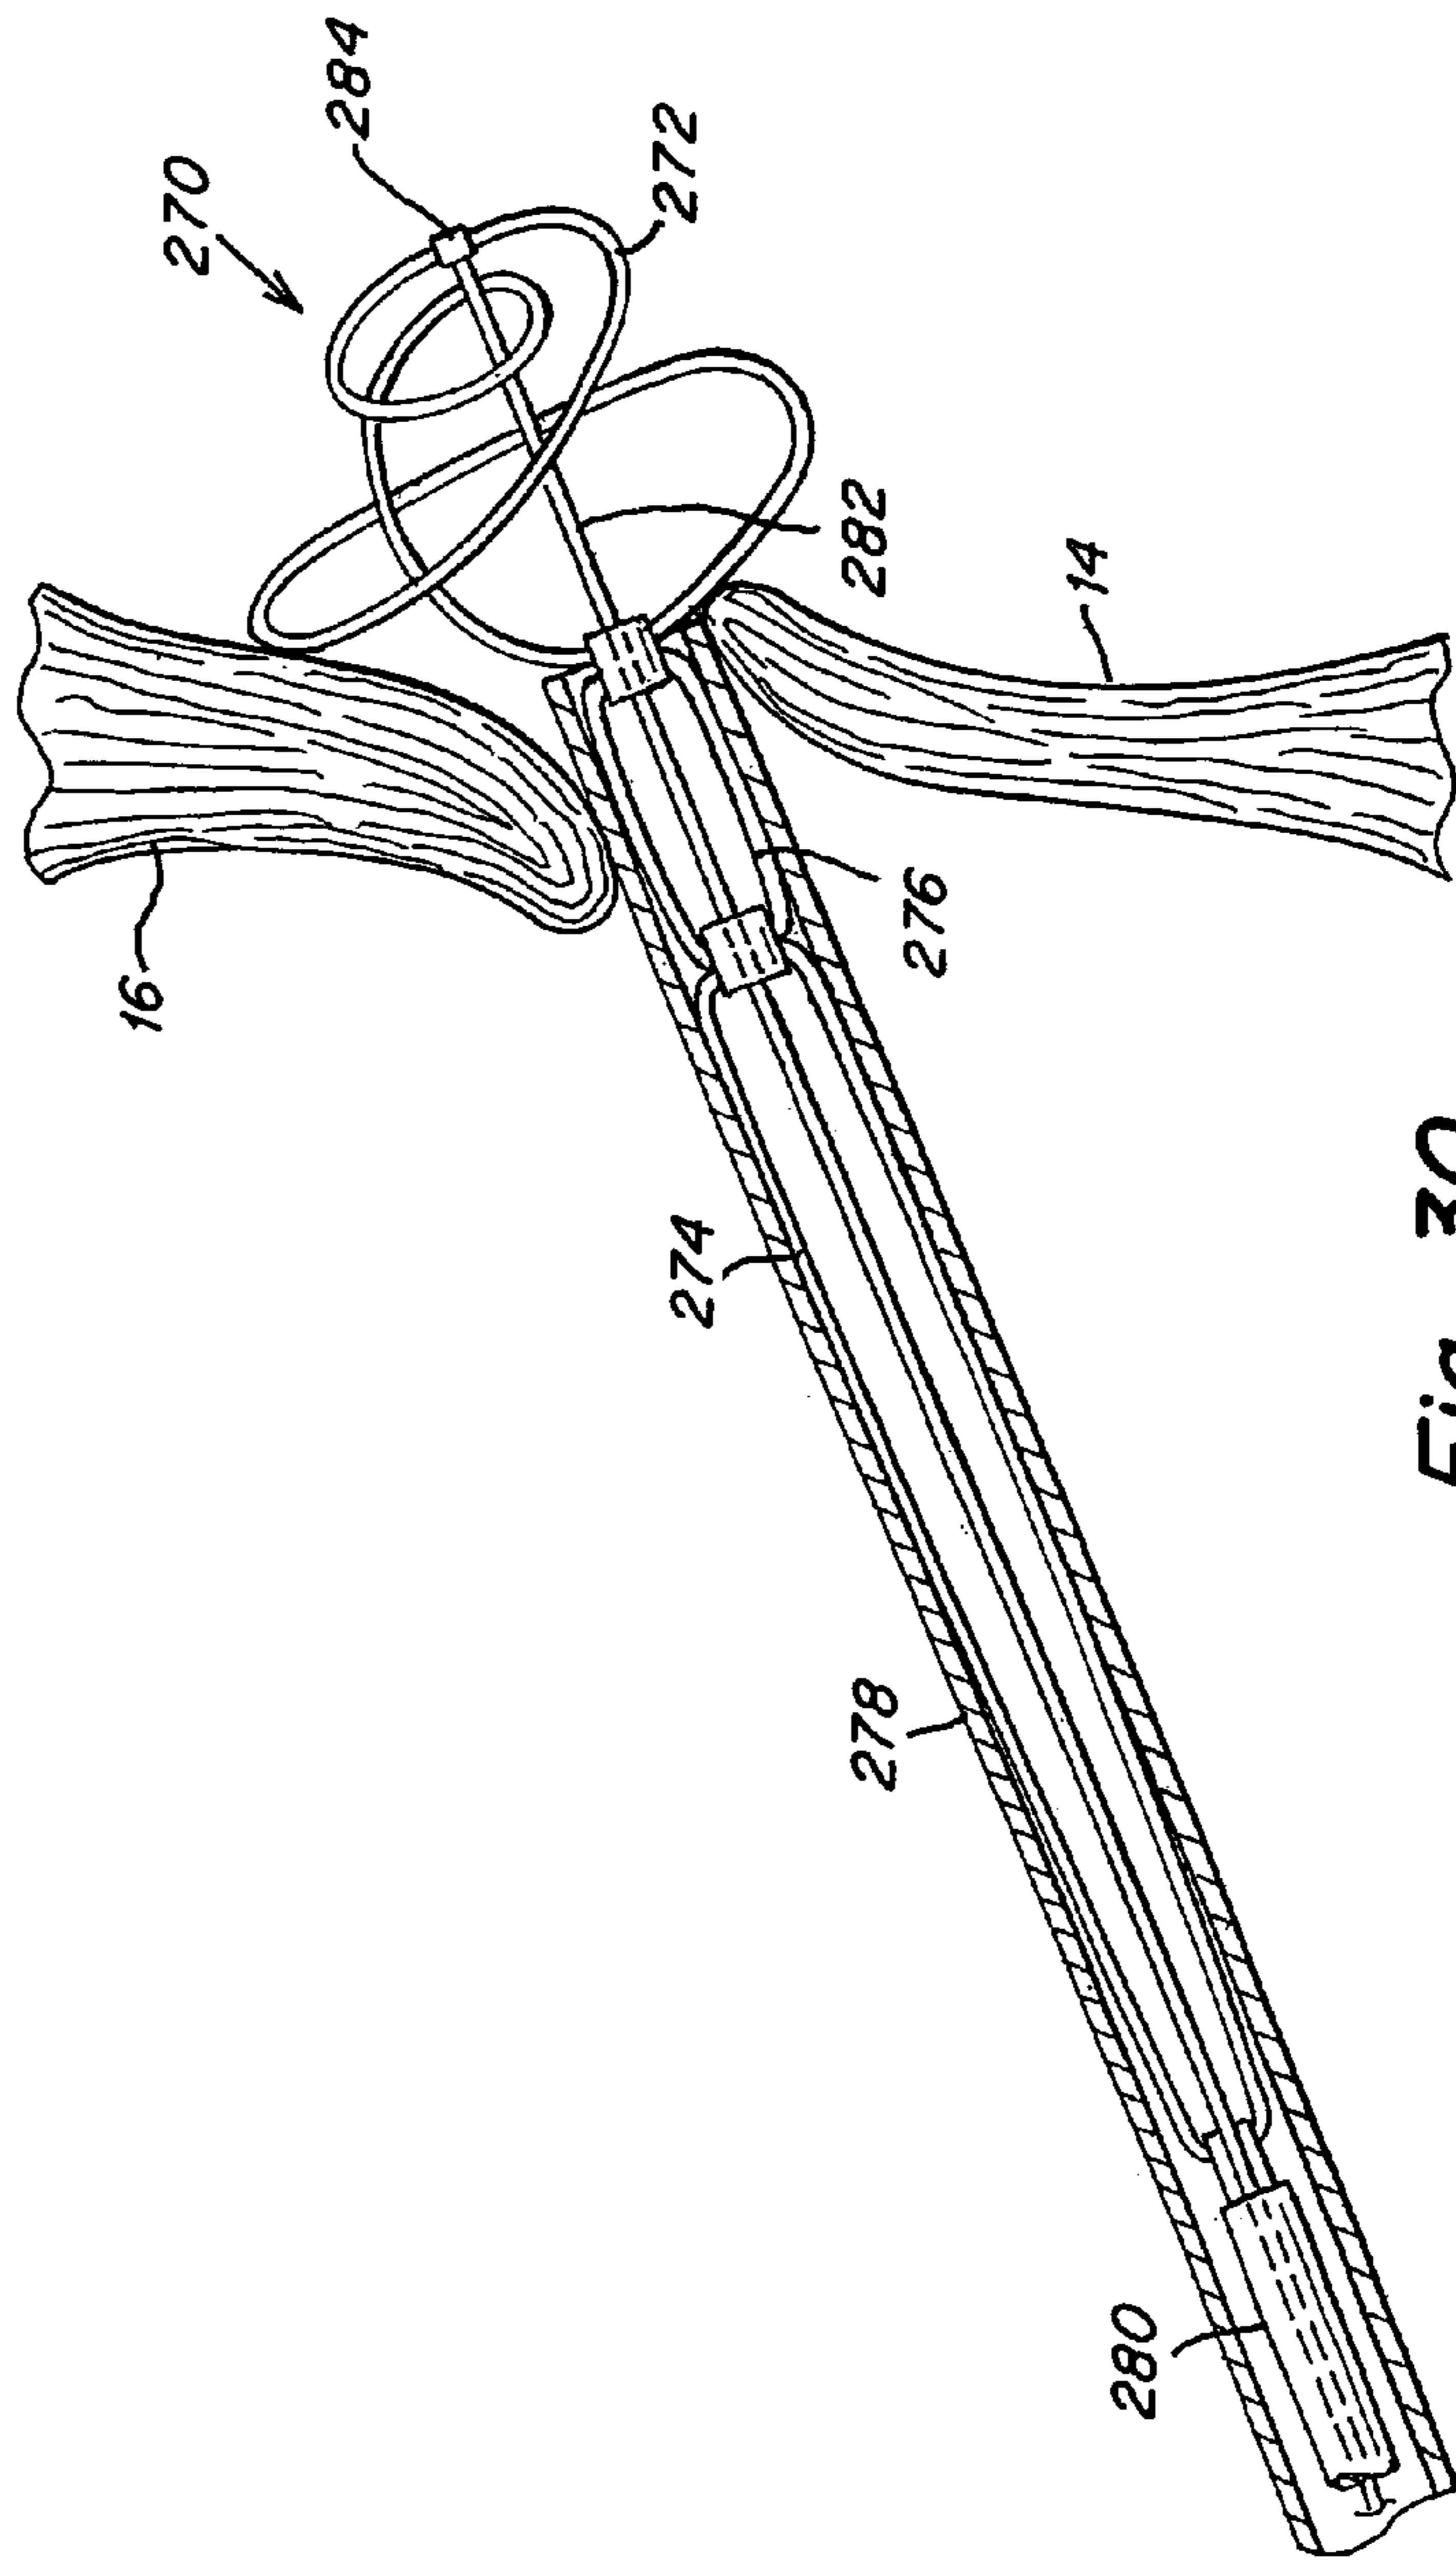


Fig. 30

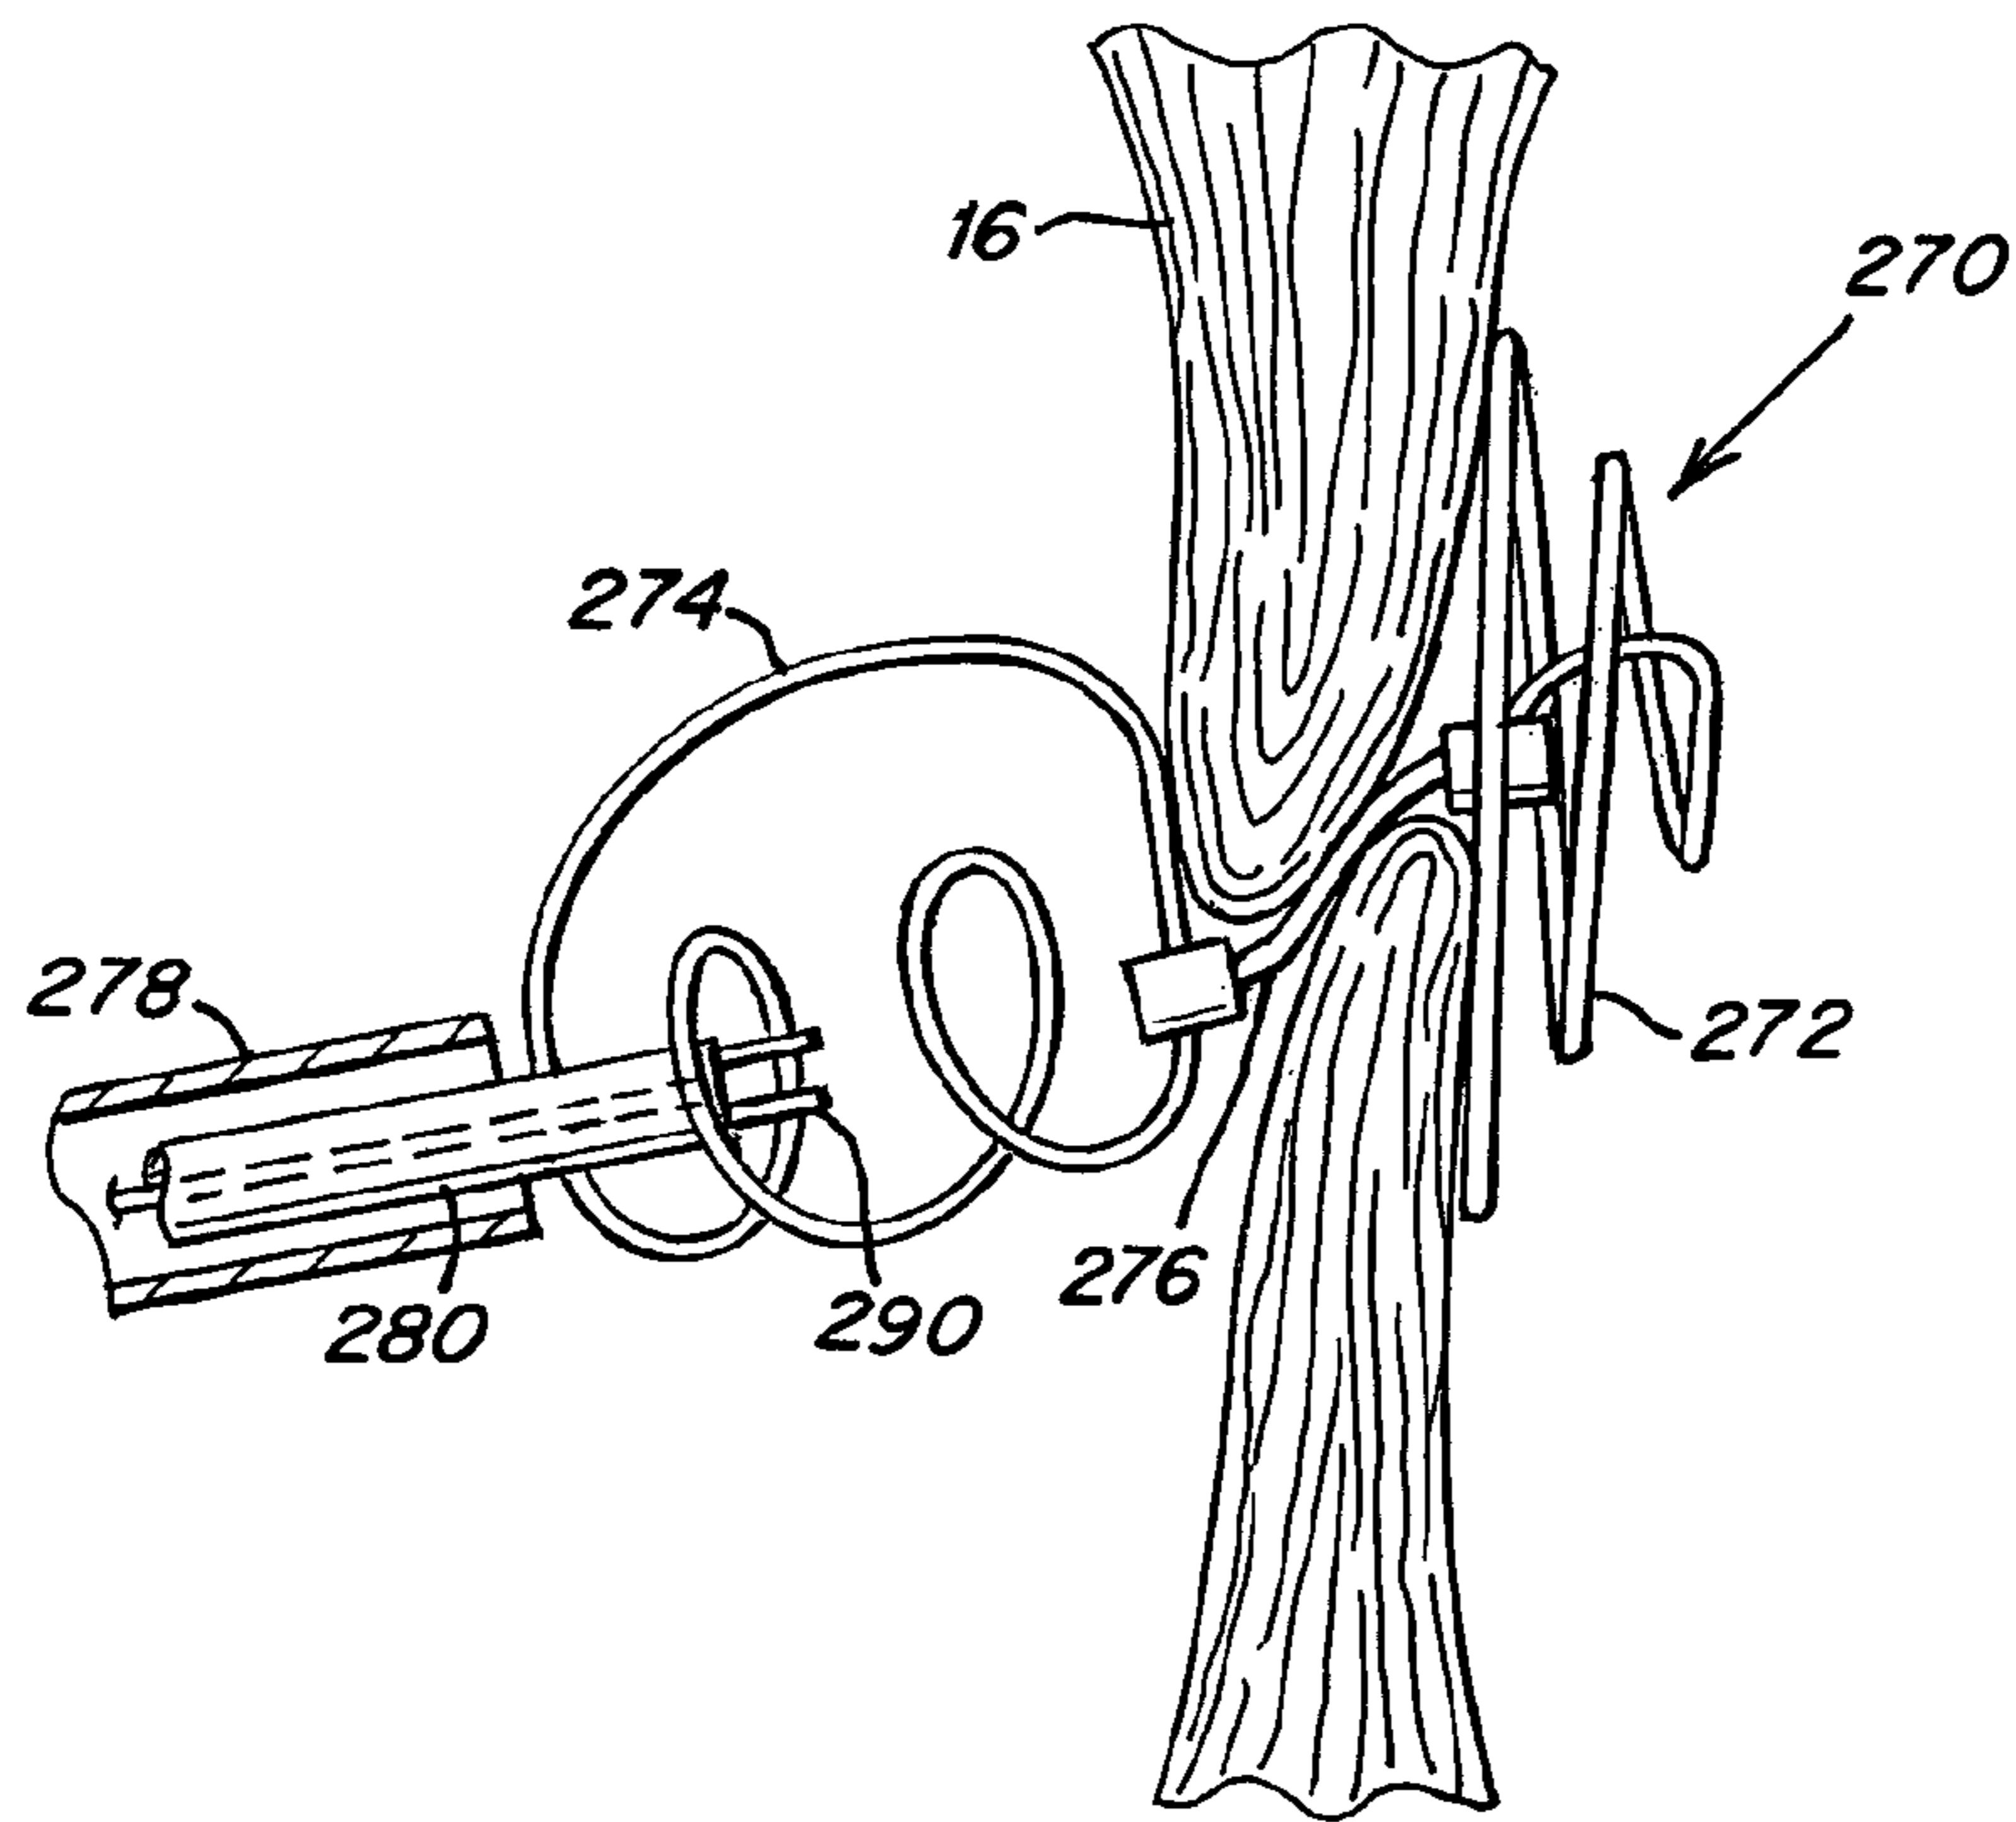


Fig. 31

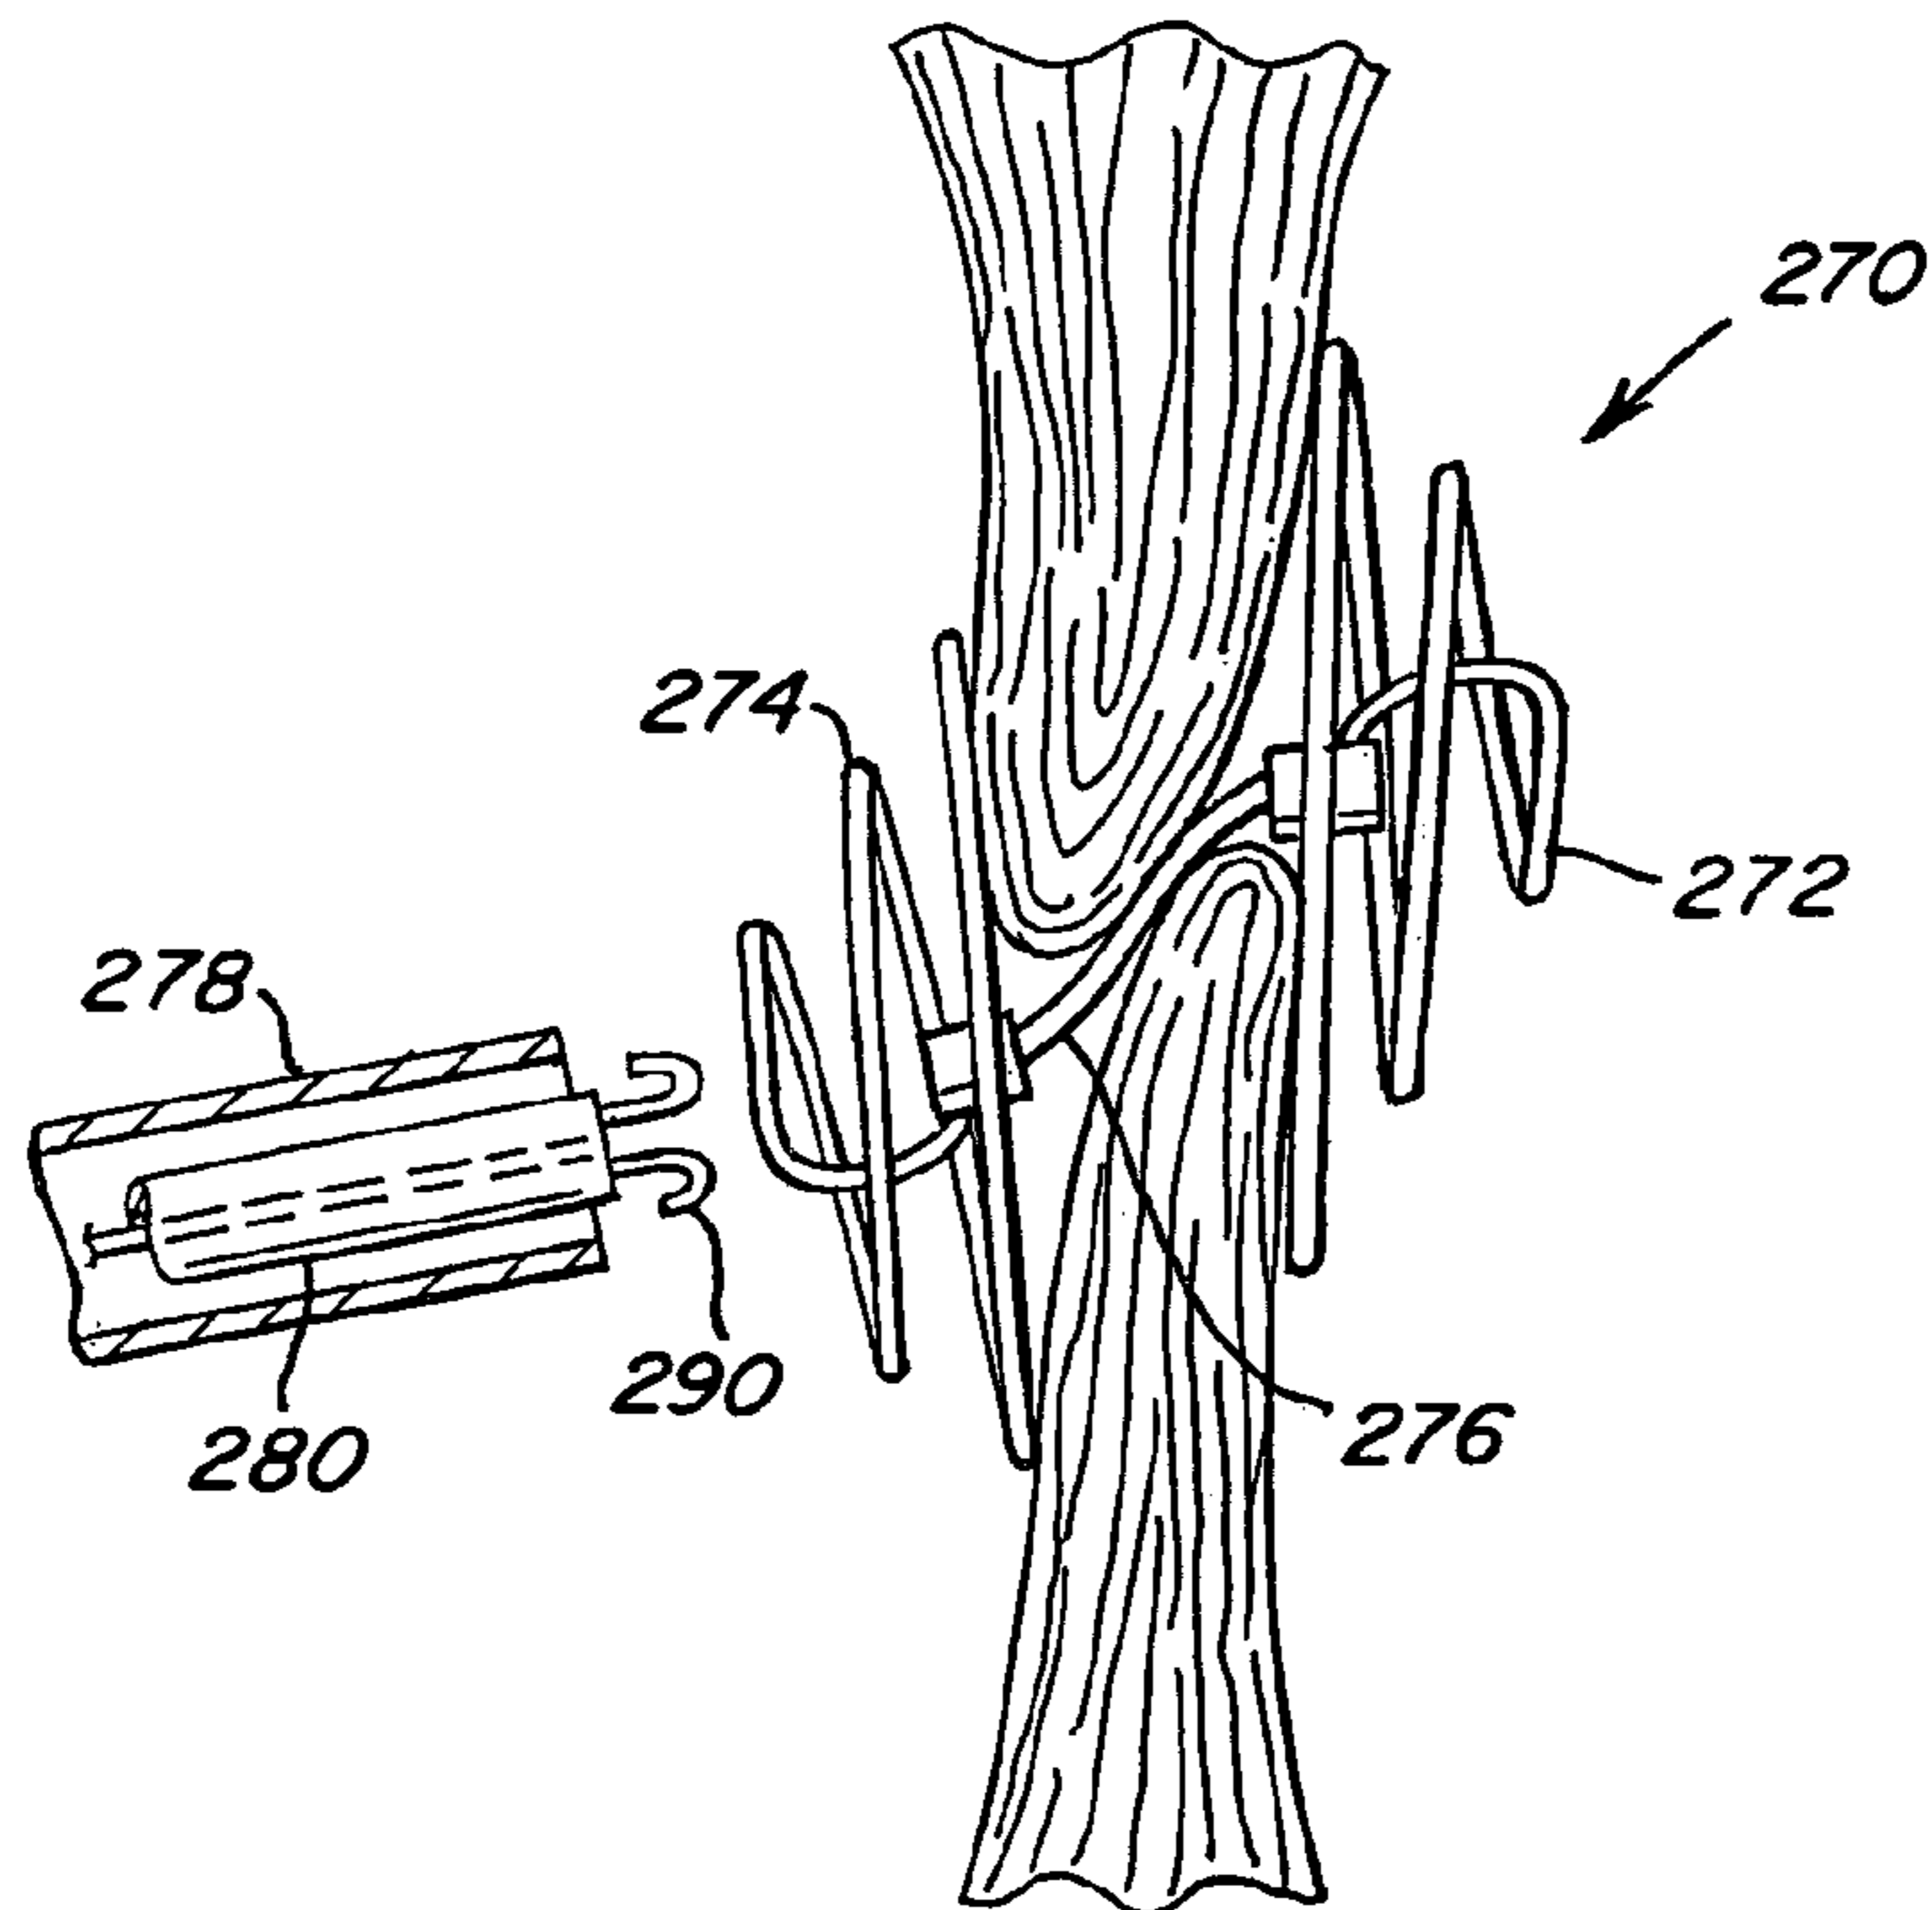


Fig. 32

1

DOUBLE COIL OCCLUDER

CROSS-REFERENCE TO RELATED
APPLICATION

This application claims priority from provisional Ser. No. 60/568,526, filed May 6, 2004, which is incorporated herein by reference.

BACKGROUND

This invention relates to an occluder for closing a septal defect.

A PFO, illustrated in FIG. 1, is a persistent, one-way, usually flap-like opening in the wall between the right atrium 10 and left atrium 12 of the heart. Because left atrial pressure is normally higher than right atrial pressure, the flap formed by septum primum 14 and septum secundum 16 usually stays closed. Under certain conditions, however, right atrial pressure can exceed left atrial pressure, which creates the possibility that blood could pass from the right atrium to the left atrium through a PFO tunnel 18 and allow blood clots to enter the systemic circulation. It is desirable to avoid this situation.

SUMMARY

Embodiments of the present invention relate to an occluder that has a coil on one or both sides of a medical defect, particularly a septal defect such as a patent foramen ovale (PFO). Each coil is preferably provided as a tube that is hollow, with or without a closed end. In some embodiments, the tube can be delivered over a wire.

In the case of use for occluding a PFO, the coils can be designed to provide a compressive force to one or both of septum primum and septum secundum of a PFO. The device can further include a tissue scaffold.

Other features and advantages will become apparent from the following detailed description and drawings.

DESCRIPTION OF THE DRAWINGS

FIG. 1 is a cross-sectional view showing a patent foramen ovale (PFO).

FIGS. 2A, 2B, 3A, 3B, and 4 are various side, end, and perspective views of a device according to a first embodiment of the present invention.

FIGS. 5-8 are partial side and partial cross-sectional views showing delivery of the device of the type shown in FIG. 4.

FIGS. 9 and 10 are perspective views of additional embodiments of a device according to the present invention.

FIGS. 11-16 are perspective, plan, end, and side views of an occluder according to another embodiment of the present invention.

FIGS. 17 and 18 are perspective views of another embodiment of the present invention, which is a variation of the embodiment of FIG. 11.

FIGS. 19 and 20, and FIGS. 21 and 22 are perspective views of two additional embodiments of the present invention.

FIGS. 23-26 are partial cross-sectional, partial side views of a device of the type shown in FIG. 22 being delivered to a PFO.

FIG. 27 is a perspective view of another embodiment of the present invention showing coils with outer ends rigidly connected to a center joint.

FIG. 28 is a perspective view showing the device of FIG. 27 in a partially stretched form for loading into a catheter.

2

FIGS. 29-32 are partial side, partial cross-sectional views showing the delivery of the device of the type shown in FIGS. 27 and 28.

DETAILED DESCRIPTION

The present invention relates to embodiments of a septal occluder with one or two spiral coils, including a double spiral coil embodiment. The coils are preferably hollow with open or closed ends, and either or both are designed to provide a compressive force when deployed in a septal defect, such as a PFO. While the coils are preferably formed from hollow tubes that can increase the strength of the spirals over solid wires, solid wires could be used. The hollow tubes may also be easier to deliver, and can be provided over a wire. Another double spiral coil design is shown in provisional application Ser. No. 60/528,022, filed Dec. 9, 2003, and in the nonprovisional Ser. No. 11/008,539, filed Dec. 9, 2004, each of which is expressly incorporated by reference.

Referring to FIGS. 2A-4, in this embodiment, an occluder 20 has two coils, a proximal (right atrial) coil 22 and a distal (left atrial) coil 24. These coils are coupled together through a center joint 26. This center joint has a first collar 28 at an inner end of coil 22, a second collar 30 at an inner end of coil 24, and connecting rods 32 and 34 coupling collars 28 and 30. As indicated in FIGS. 2B and 3A, rods 32 and 34 are preferably in a horizontal plane in a position shown in FIG. 4 in a manufactured and non-deployed position.

Referring to FIG. 3B, when occluder 20 is in the deployed position in a PFO, coils 22 and 24 each have an upper portion in contact with septum secundum 16 and a lower portion in contact with septum primum 14. As is also indicated, rods 32 and 34 and center joint 26 can extend side-by-side in, and conform to, the geometry of the PFO tunnel between septum primum 14 and septum secundum 16.

The coils can be made from a number of different materials, including metal or nonmetal. Among nonmetals, a preferable material is a polymer, which can be a bioresorbable polymer. In this embodiment, the ends of the coils are shown as being open, but one or both of the ends could be closed, either with a solid piece or with a mesh. In this embodiment, the coils spiral outwardly from a central location.

As shown in FIG. 5, the device with coils in the form of hollow tubes can be mounted over a wire 36 that extends through an inner catheter 38. Wire 36 and catheter 38 are both in a delivery sheath 40. The device with coil 24, coil 22, and center joint 26 is in a substantially elongated and a low profile configuration, such that they fit into a sheath that is preferably 10 French or smaller, although a larger sheath could be used.

As shown in FIG. 5, sheath 40 is inserted into the left atrium. Referring to FIG. 6, sheath 40 and wire 36 are retracted, while inner catheter 38 is maintained in its current position to hold the position of coil 24. These relative movements, which can be at the same or at different rates, allow coil 24 to be released from delivery sheath 40 and into the left atrium. The coil is preferably formed from a material with good shape memory properties so that it returns to its coil form when released from sheath 40. Such a material is especially useful when the coil has a free outer end not connected to anything else.

Referring to FIGS. 7 and 8, sheath 40 and wire 36 are retracted further while inner catheter 38 is used to help maintain conduit 22 in a desired position. With such further removal, the center joint is positioned within the PFO tunnel, and coil 22 is allowed to resume its coil shape on the right atrial side of the PFO.

The device is formed with suitable materials, dimensions, and configuration so that the coils provide enough compressive force to hold together septum primum and septum secundum sufficiently to prevent clots from passing from the right atrial side to the left atrial side. As will be apparent below, while occluder **20** has a spiral that is connected to a center joint and spirals outwardly (i.e., with an increasing radius) to a free end, in other embodiments, the coil spirals inwardly from the center joint and may have an end that is connected to the center joint. In this embodiment and others, the outer surface can be roughened to produce an inflammatory effect to encourage healing. In this embodiment and others, a single coil can be used on one side of the defect, with another structure, such as an umbrella-shaped structure on the other side of the defect.

FIG. **9** is a perspective view of another embodiment of the present invention in which a device **90** is formed from a single, monolithic hollow tube shaped to form a distal coil **94**, a proximal coil **92**, and a connecting segment **96** that extends from the inner ends of coils **92** and **94**. If desired, portions of device **90**, such as at connecting segment **96**, can have whiskers that can be formed by gluing short threads of the material used to make the tube or some other material, or connecting segment **96** can be partially shaved or otherwise frayed. The use of whiskers can serve as an inflammatory agent that encourages healing. While mentioned here, whiskers could be used in other embodiments.

Like the embodiment of FIG. **2a**, the inner ends (i.e., smaller radius portion) of the coils are coupled to a connector or transition to a connecting segment, and the outer ends of the coils are free and are not connected to any other structure.

Referring to FIG. **10**, in another embodiment of the present invention, a device **100** has a proximal coil **102** and distal coil **104**. In this case, one of the coils, in this case coil **102**, starts spiraling from the inside where there is a free end, and spirals out with increasing radius to an outer end of coil **102** where the coil is then curved away from the plane of the spiral and is connected to a collar **108** of a center joint **106**. Distal coil **104** is shaped in a similar manner.

As is further indicated in FIG. **10**, a tissue scaffold **109** can be incorporated into center joint **106**. The scaffold is connected between the collars and can be bounded by the connecting rods between the collars, although it could be used at other locations instead of this location or additionally at other locations. While shown between the connecting rods, it can extend around the connecting rods and/or around other portions of the device to encapsulate them. The tissue scaffold promotes encapsulation and endothelialization, thereby further encouraging anatomical closure of septum primum and septum secundum. While shown just in FIG. **10**, a tissue scaffold can be incorporated into other embodiments.

A tissue scaffold can be formed of any flexible, biocompatible material capable of promoting tissue growth, including but not limited to polyester fabrics, Teflon-based materials, such as ePTFE, polyurethanes, metallic materials, polyvinyl alcohol (PVA), extracellular matrix (ECM) or other bioengineered materials, synthetic bioresorbable polymeric scaffolds, other natural materials (e.g. collagen), or combinations of these materials. A tissue scaffold or the spiral or center joint can have drugs or biological agents to improve the defect healing process and/or to prevent clotting.

Referring to FIGS. **11-16**, a device **110** according to still another embodiment can have close-ended hollow or solid spirals, and can have a free end of a coil on one or both sides of a defect locked to a center joint (FIG. **11**) or unlocked (FIG. **12**). By locking one or both free ends of a spiral to a center

joint, the clamping force of the device can be increased relative to a device with a free end.

A center joint **116** has a latching loop **120** connected to an outer end of coil **114**. From the inner end of coil **114**, there is a free end **128** that can extend a short distance through loop **120**. Similarly, coil **112** has an outer end attached to a latching loop **118** and an inner end that extends to a free end **130** that extends a short distance through the opening in loop **118**. Free ends **128** and **130** each have a bent end that extends through latching loops **118** and **120** in a manner that they stay in the latched position. Latching loops **118** and **120** are connected together with connecting rods **122** and **124**.

Additional views of this device are shown in FIGS. **13-15** and in FIG. **16** which shows the device as deployed. FIG. **15**, in particular, shows how the latching loops **118** and **120** are coupled to the outer ends of the spiral, the spirals extend inwardly, and at the inner end of the spiral, a free end **128**, **130** extends to the latching loop on each side. As is also shown in FIG. **16**, the connecting rods **122** and **124** (not shown) have some ability to bend and conform to the geometry of the PFO tunnel, while the spirals can provide a compressive force between septum primum and septum secundum.

FIGS. **17** and **18** show an embodiment of a device **170** that is similar to that in FIGS. **11** and **12**, except that rather than having free ends extending a short way through loops and held in the loops with bent ends, it has locks, such as magnetic locks, **172**, **174** on the free ends. In this case, the free end has one magnetic piece and the center joint has another magnet and a conforming mechanical structure, such as a short lug and an opening for receiving the lug.

Referring to FIGS. **19** and **20**, a device **190** has features of several of the embodiments above. The device has a proximal coil **192** and a distal coil **194** connected together through a center joint **196** that includes collars **198** and **199**. Coil **192** is rigidly connected to a side of collar **198** from where it extends radially outwardly and then spirals inwardly until at an inner part of the spiral, it bends toward the center. At the center, there is a bent end that can extend through collar **198** to hold it in place. In this case, the interior end of the loop has a bent end for engaging the collar, but it could have the reverse form with the inner end of the spiral connected to the collar and the outer end of the spiral curved to extend through the collar. Coil **194** in this embodiment is similarly connected to the other side of the device, although the different coils can have different structures.

FIG. **20** shows device **190** of FIG. **19** with the inner ends of the coils detached from the respective collars.

FIGS. **21** and **22** show embodiments similar to those in FIGS. **19** and **20**, except that the connection between the spiral and the center joint has a snap fit to hold them together. The device is shown with the center joint and spiral detached in FIG. **22**. In this case, like the embodiment of FIGS. **19** and **20**, the coil spirals inwardly from the outside to a lock, but it could have the reverse form of spiral.

FIGS. **23-26** show the delivery of a device of the type shown in FIGS. **21** and **22**. FIG. **23** shows the device of FIG. **21** loaded into a sheath **230**, and coupled to a mandrel **240** and a delivery catheter **242**. As shown herein, the device has a small profile, preferably small enough to fit in a 10 F sheath. Referring to FIG. **24**, sheath **230** with the loaded device is provided through the PFO tunnel and into the left atrial side. Sheath **230** is then retracted while an end cap **234** of distal coil **232** is held in place by mandrel **240** to allow a distal coil **232** and end cap **234** to be released from sheath **230**. A proximal end cap is held in place with delivery catheter **242**.

Referring to FIGS. **25** and **26**, end cap **234** coupled to collar **235**, e.g., with a snap fit, and mandrel **240** (not shown here) is

5

withdrawn. Sheath 230 is then further retracted to release a proximal coil 236 against septum primum 14 and septum secundum 16 on the right atrial side until end cap 244 is coupled to collar 246. Delivery catheter 242 is releasably detached from end cap 244, resulting in the positioned device as shown in FIG. 26. The releasable connection between catheter 242 and end cap 244 can be with grappling hooks 250 (FIG. 25), which are generally known for use in delivering medical devices.

FIGS. 27 and 28 show another embodiment of the present invention similar to that shown in FIGS. 21 and 22, except that the device is shown with a center joint that has a rigid and generally non-separable connection to both coils. FIG. 28 shows the device of FIG. 27 in an elongated form as it would be loaded into a sheath for delivery. With further elongation, the profile of the device can be reduced to fit inside a delivery sheath as shown in FIG. 29.

FIGS. 30-32 show the release of the device of FIGS. 27 and 28 in the PFO tunnel. This delivery is generally similar to that described in conjunction with FIGS. 23-26. A device 270 with a distal coil 272, proximal coil 274, and center joint 276 is elongated as shown in FIG. 28 and loaded into a delivery sheath 278. A first delivery catheter 280 is releasably connected to a portion of coil 274 at a proximal end, and a second delivery catheter 282 is releasably connected to a portion of distal coil 272 with a connection 284. As shown in FIG. 30, sheath 278 is withdrawn while second delivery catheter 282 holds distal coil 272 in place so it can open into a coil on the left atrial side. As shown in FIGS. 31 and 32, sheath 278 is further retracted to allow right atrial coil 274 to open on the right atrial side. Coil 274 as shown is releasably held with hooks 290 to provide control over the release. Having described embodiments of the present invention, it should be understood that modifications can be made without departing from the scope of the invention.

What is claimed:

1. A device adapted to press together the septum primum and the septum secundum between the atrial chambers, the device comprising:

first and second clamping spirals, each having a size suitable for use on each side of the septum, wherein each of the first and second clamping spirals has a first end at an outer edge and a free end; and

a central connector for connecting the first end of the first and second clamping spirals and passing through the tunnel between the septum primum and the septum secundum,

wherein at least one of the spirals includes a length of wire extending in a radial direction from an inner portion of the spiral to the outer edge of the spiral and locking the free end of the spiral to the central connector.

2. The device of claim 1, wherein the spirals spiral outwardly from the central connector to the free ends.

3. The device of claim 1, wherein the central connector includes at least one hollow rod extending from a central region of the first spiral to a central region of the second spiral.

4. The device of claim 1, wherein the spirals and the central connector are formed from a single wire.

5. The device of claim 1, wherein at least one of the spirals has a radially extending portion extending from the central connector, the at least one spiral extends inwardly back to the central connector, and the center joint is flexible.

6

6. The device of claim 1, wherein the device is formed from a bioresorbable polymer.

7. The device of claim 1, wherein the spirals each circle around more than 360°.

8. The device of claim 1, wherein the central connector includes a scaffold for promoting tissue growth.

9. The device of claim 1, wherein the first end of each of the first and second spirals includes a radial portion connected to the central connector.

10. The device of claim 1, wherein the central connector has an opening at least one end, and the free end of at least one of the spirals is adapted to extend through the opening to form a connection.

11. The device of claim 9, wherein the central connector and the second end have a snap-fit connection.

12. The device of claim 1, wherein the first spiral spirals outwardly from the central connector and extends from an outermost point radially back to the central connector where the radial portion is connected to the central connector.

13. The device of claim 12, wherein the radial portion is detachably connected to the central connector.

14. The device of claim 12, wherein the radial portion is non-detachably connected to the central connector.

15. A device adapted to be disposed in a patent foramen ovale tunnel and comprising first and second separate spirals and a connecting member together connected to the spirals with respective first and second joints, wherein each spiral has one end at an outer edge connected to one of the first and second joints, and a second end connectible to the respective first or second joint, the spirals forming closed loops when the second end is connected.

16. The device of claim 15, wherein the spirals spiral outwardly from the first and second joints and have a radial portion extending inwardly from an outermost part of a spiral.

17. The device of claim 15, wherein the connecting member includes two wires extending between the first and second joints.

18. The device of claim 15, further comprising a membrane attached to the connecting member for promoting tissue growth.

19. The device of claim 15, wherein the first and second joints have an opening for the second end to extend through.

20. The device of claim 15, wherein the first and second joints have snap fit connectors for connection to the respective second ends.

21. A method comprising introducing into a patent foramen ovale (PFO) the device of claim 1.

22. The method of claim 21, wherein the introducing includes first providing a wire into the body, and then providing the device over the wire.

23. The method of claim 22, wherein the method includes loading the device into a sheath, providing a catheter to limit movement of the device in the proximal direction, and providing the catheter, device, and sheath to the region near the PFO.

24. The method of claim 23, further comprising extending the sheath and device through a PFO tunnel to a left atrium, limiting movement of the device in the proximal direction, and withdrawing the sheath in the proximal direction to release the second spiral on the left atrium side of the PFO.

25. The method of claim 24, further comprising further withdrawing the sheath in the proximal direction.

* * * * *