



US007886419B2

(12) **United States Patent**  
**Huang et al.**

(10) **Patent No.:** **US 7,886,419 B2**  
(45) **Date of Patent:** **Feb. 15, 2011**

(54) **STENT CRIMPING APPARATUS AND METHOD**

(75) Inventors: **Bin Huang**, Pleasanton, CA (US); **David C. Gale**, San Jose, CA (US); **Daniel Castro**, Santa Clara, CA (US)

(73) Assignee: **Advanced Cardiovascular Systems, Inc.**, Santa Clara, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1113 days.

(21) Appl. No.: **11/489,309**

(22) Filed: **Jul. 18, 2006**

(65) **Prior Publication Data**

US 2008/0016668 A1 Jan. 24, 2008

(51) **Int. Cl.**

**G01M 19/00** (2006.01)

**B23Q 3/00** (2006.01)

(52) **U.S. Cl.** ..... **29/407.08**; 29/515; 29/516; 29/283

(58) **Field of Classification Search** ..... 29/407.08, 29/407.09, 407.1, 505, 515, 516, 282, 283, 29/283.5

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,687,135 A 8/1972 Stroganov et al.  
3,839,743 A 10/1974 Schwarcz  
3,900,632 A 8/1975 Robinson  
4,104,410 A 8/1978 Malecki  
4,110,497 A 8/1978 Hoel  
4,321,711 A 3/1982 Mano

4,346,028 A 8/1982 Griffith  
4,596,574 A 6/1986 Urist  
4,599,085 A 7/1986 Riess et al.  
4,612,009 A 9/1986 Drobnik et al.  
4,633,873 A 1/1987 Dumican et al.  
4,656,083 A 4/1987 Hoffman et al.  
4,718,907 A 1/1988 Karwoski et al.  
4,722,335 A 2/1988 Vilasi  
4,723,549 A 2/1988 Wholey et al.  
4,732,152 A 3/1988 Wallstén et al.  
4,733,665 A 3/1988 Palmaz  
4,739,762 A 4/1988 Palmaz  
4,740,207 A 4/1988 Kreamer  
4,743,252 A 5/1988 Martin, Jr. et al.  
4,768,507 A 9/1988 Fischell et al.  
4,776,337 A 10/1988 Palmaz

(Continued)

FOREIGN PATENT DOCUMENTS

DE 44 07 079 9/1994

(Continued)

OTHER PUBLICATIONS

International Search Report for PCT/US2007/016200, filed Jul. 17, 2007, mailed Nov. 21, 2007, 5 pgs.

(Continued)


Primary Examiner—Essama Omgba

(74) Attorney, Agent, or Firm—Suire, Sanders & Dempsey LLP.

(57) **ABSTRACT**

A method for crimping a stent onto a balloon includes inflating a balloon with a fluid, sliding a stent over the inflated balloon, crimping the stent onto the balloon, and controlling the pressure inside the balloon below a given value when the stent is being crimped onto the balloon.

**21 Claims, 3 Drawing Sheets**

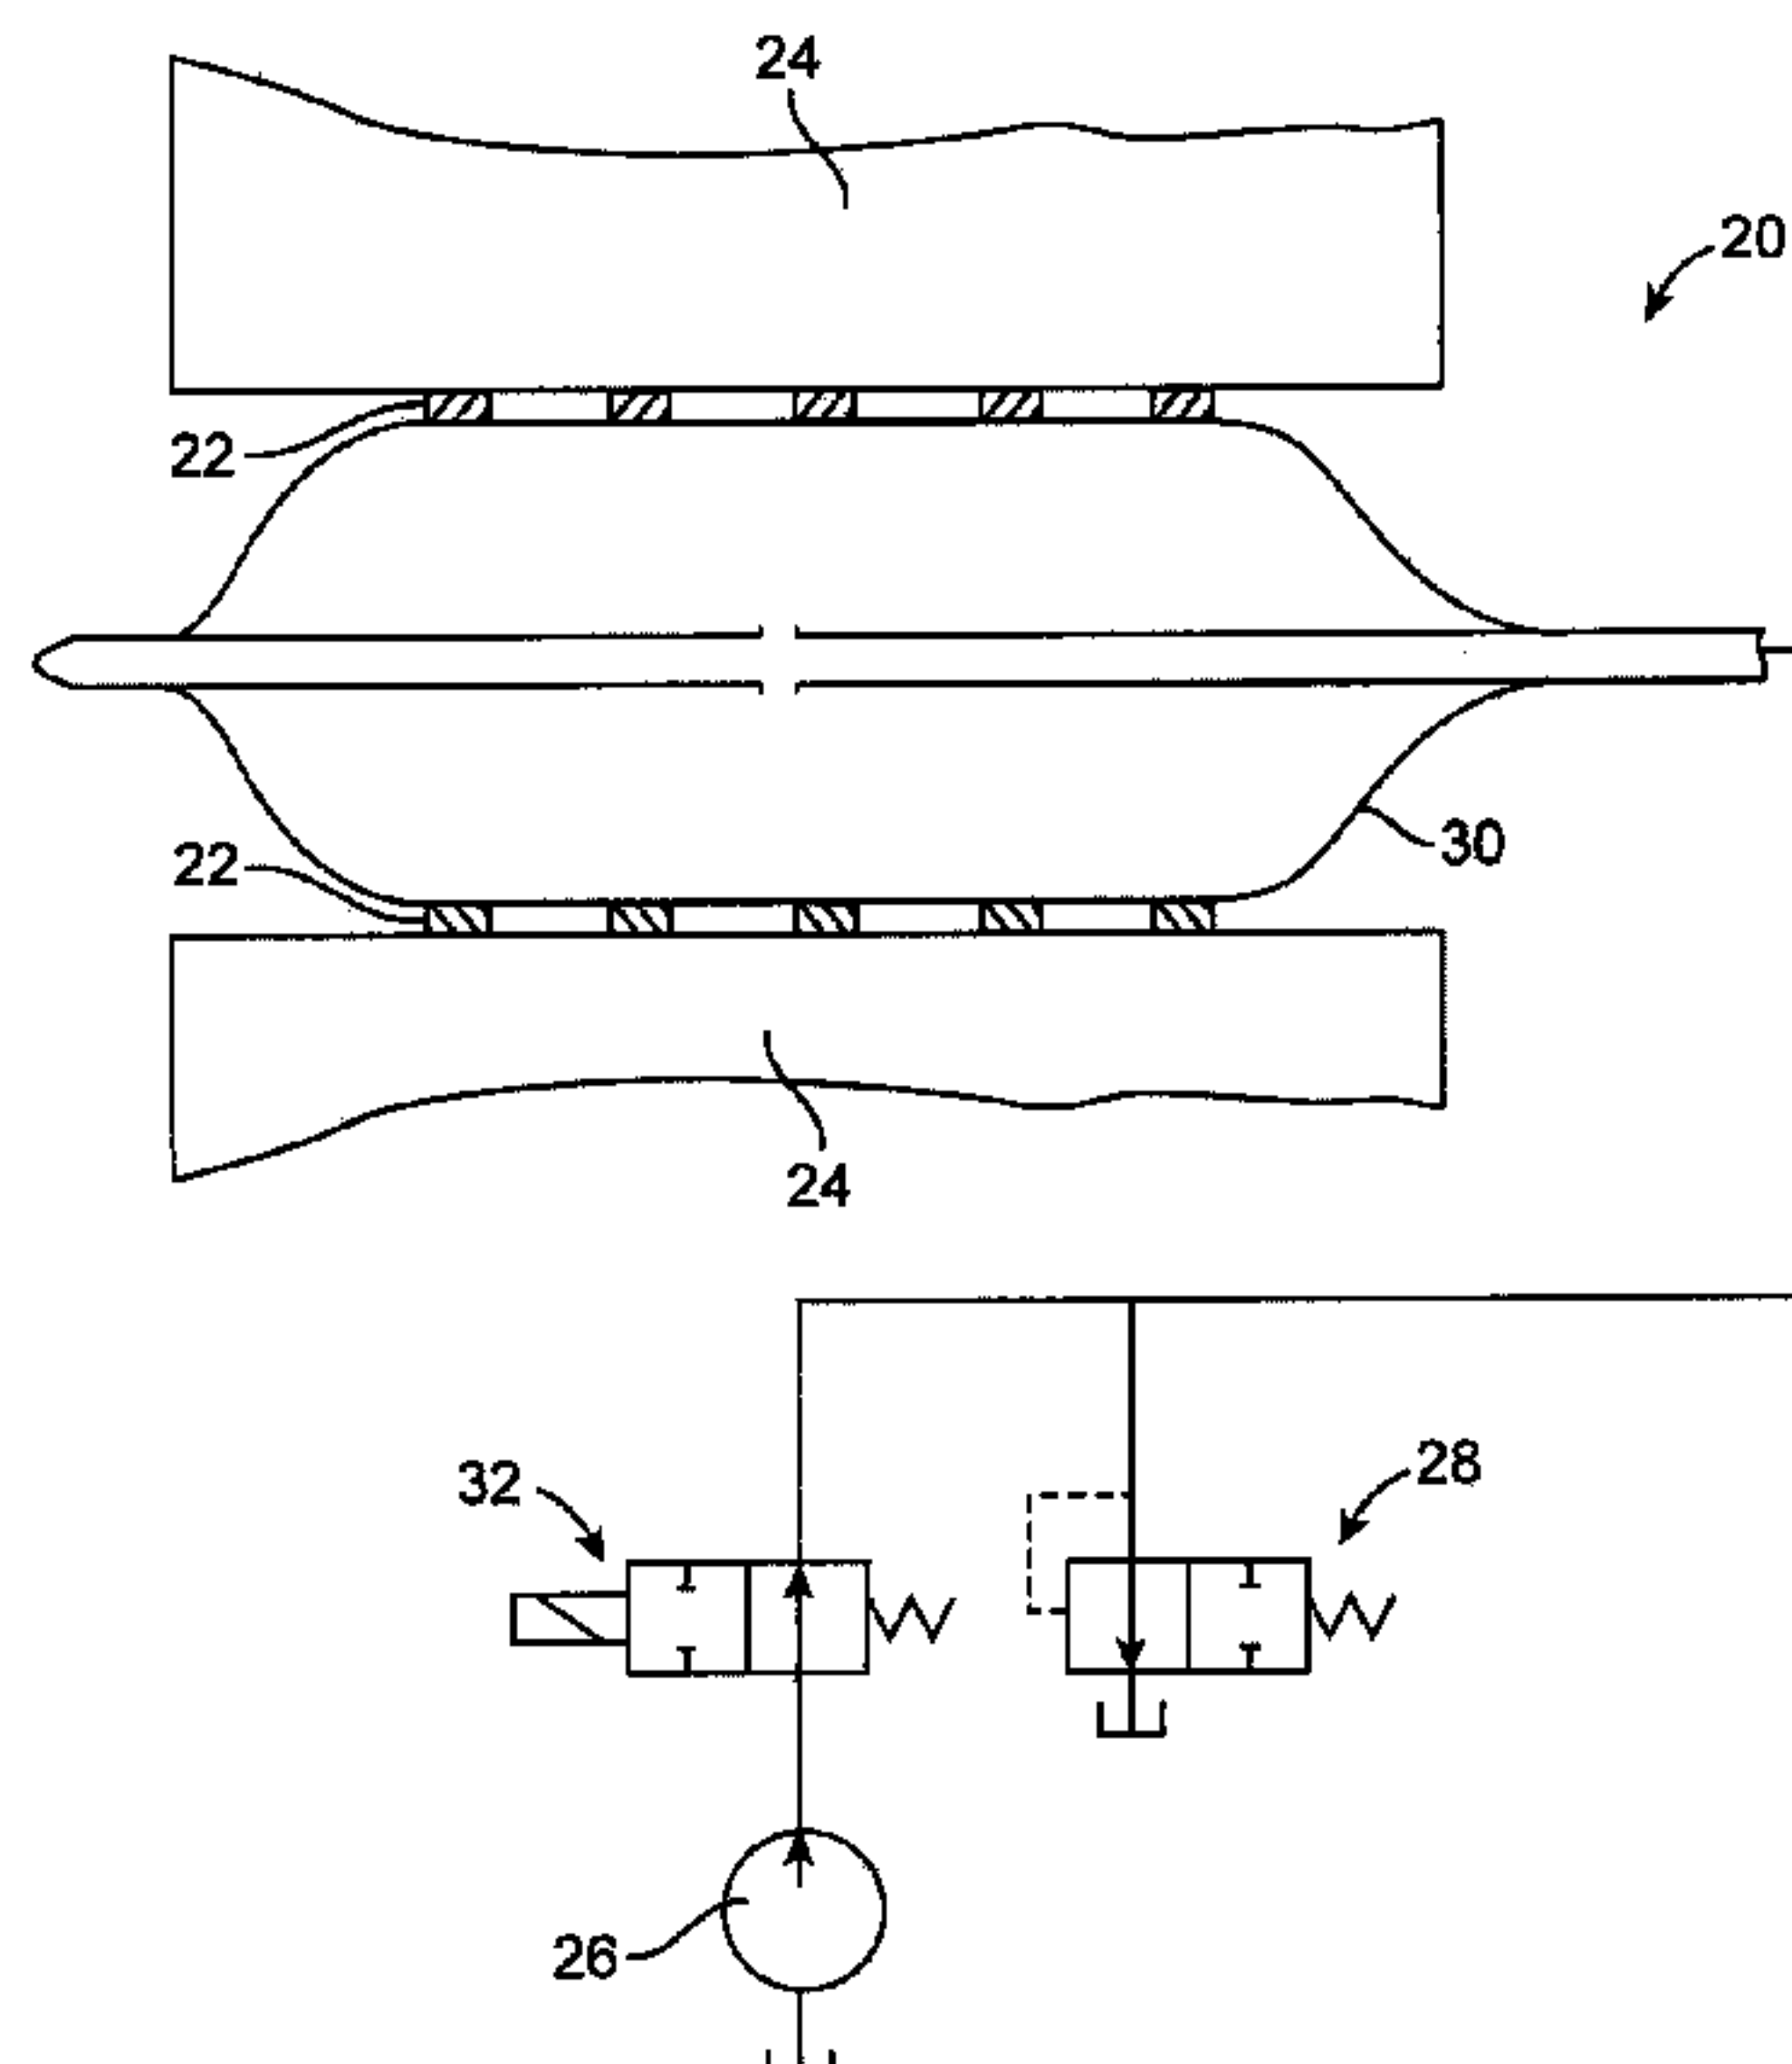

U.S. PATENT DOCUMENTS					
4,800,882	A	1/1989	Gianturco	5,599,922	A 2/1997 Gryaznov et al.
4,816,339	A	3/1989	Tu et al.	5,605,696	A 2/1997 Eury et al.
4,818,559	A	4/1989	Hama et al.	5,607,442	A 3/1997 Fischell et al.
4,850,999	A	7/1989	Planck	5,607,467	A 3/1997 Froix
4,877,030	A	10/1989	Beck et al.	5,618,299	A 4/1997 Khosravi et al.
4,878,906	A	11/1989	Lindemann et al.	5,629,077	A 5/1997 Turnlund et al.
4,879,135	A	11/1989	Greco et al.	5,631,135	A 5/1997 Gryaznov et al.
4,886,062	A	12/1989	Wiktor	5,632,771	A 5/1997 Boatman et al.
4,902,289	A	2/1990	Yannas	5,632,840	A 5/1997 Campbell
4,977,901	A	12/1990	Ofstead	5,637,113	A 6/1997 Tartaglia et al.
4,994,298	A	2/1991	Yasuda	5,649,977	A 7/1997 Campbell
5,019,090	A	5/1991	Pinchuk	5,667,767	A 9/1997 Greff et al.
5,028,597	A	7/1991	Kodama et al.	5,667,796	A 9/1997 Otten
5,059,211	A	10/1991	Stack et al.	5,670,558	A 9/1997 Onishi et al.
5,062,829	A	11/1991	Pryor et al.	5,693,085	A 12/1997 Buirge et al.
5,084,065	A	1/1992	Weldon et al.	5,700,286	A 12/1997 Tartaglia et al.
5,085,629	A	2/1992	Goldberg et al.	5,707,385	A 1/1998 Williams
5,100,429	A	3/1992	Sinofsky et al.	5,711,763	A 1/1998 Nonami et al.
5,104,410	A	4/1992	Chowdhary	5,716,981	A 2/1998 Hunter et al.
5,108,417	A	4/1992	Sawyer	5,725,549	A 3/1998 Lam
5,108,755	A	4/1992	Daniels et al.	5,726,297	A 3/1998 Gryaznov et al.
5,112,457	A	5/1992	Marchant	5,728,751	A 3/1998 Patnaik
5,123,917	A	6/1992	Lee	5,733,326	A 3/1998 Tomonto et al.
5,147,385	A	9/1992	Beck et al.	5,733,330	A 3/1998 Cox
5,156,623	A	10/1992	Hakamatsuka et al.	5,733,564	A 3/1998 Lehtinen
5,163,951	A	11/1992	Pinchuk et al.	5,733,925	A 3/1998 Kunz et al.
5,163,952	A	11/1992	Froix	5,741,881	A 4/1998 Patnaik
5,163,958	A	11/1992	Pinchuk	5,756,457	A 5/1998 Wang et al.
5,167,614	A	12/1992	Tessmann et al.	5,756,476	A 5/1998 Epstein et al.
5,192,311	A	3/1993	King et al.	5,765,682	A 6/1998 Bley et al.
5,197,977	A	3/1993	Hoffman, Jr. et al.	5,766,204	A 6/1998 Porter et al.
5,234,456	A	8/1993	Silvestrini	5,766,239	A 6/1998 Cox
5,234,457	A	8/1993	Andersen	5,766,710	A 6/1998 Turnlund et al.
5,236,447	A	8/1993	Kubo et al.	5,769,883	A 6/1998 Buscemi et al.
5,279,594	A	1/1994	Jackson	5,780,807	A 7/1998 Saunders
5,282,860	A	2/1994	Matsuno et al.	5,800,516	A 9/1998 Fine et al.
5,289,831	A	3/1994	Bosley	5,811,447	A 9/1998 Kunz et al.
5,290,271	A	3/1994	Jernberg	5,824,049	A 10/1998 Ragheb et al.
5,292,321	A	3/1994	Lee	5,830,178	A 11/1998 Jones et al.
5,306,286	A	4/1994	Stack et al.	5,830,461	A 11/1998 Billiar
5,306,294	A	4/1994	Winston et al.	5,830,879	A 11/1998 Isner
5,328,471	A	7/1994	Slepian	5,833,651	A 11/1998 Donovan et al.
5,330,500	A	7/1994	Song	5,834,582	A 11/1998 Sinclair et al.
5,342,348	A	8/1994	Kaplan	5,836,962	A 11/1998 Gianotti
5,342,395	A	8/1994	Jarrett et al.	5,836,965	A 11/1998 Jendersee et al.
5,342,621	A	8/1994	Eury	5,837,313	A 11/1998 Ding et al.
5,356,433	A	10/1994	Rowland et al.	5,837,835	A 11/1998 Gryaznov et al.
5,383,925	A	1/1995	Schmitt	5,840,083	A 11/1998 Braach-Maksvytis
5,385,580	A	1/1995	Schmitt	5,851,508	A 12/1998 Greff et al.
5,389,106	A	2/1995	Tower	5,853,408	A 12/1998 Muni
5,399,666	A	3/1995	Ford	5,854,207	A 12/1998 Lee et al.
5,423,885	A	6/1995	Williams	5,855,612	A 1/1999 Ohthuki et al.
5,441,515	A	8/1995	Khosravi et al.	5,855,618	A 1/1999 Patnaik et al.
5,443,458	A	8/1995	Eury et al.	5,858,746	A 1/1999 Hubbell et al.
5,443,500	A	8/1995	Sigwart	5,865,814	A 2/1999 Tuch
5,455,040	A	10/1995	Marchant	5,868,781	A 2/1999 Killion
5,464,650	A	11/1995	Berg et al.	5,873,904	A 2/1999 Ragheb et al.
5,502,158	A	3/1996	Sinclair et al.	5,874,101	A 2/1999 Zhong et al.
5,514,379	A	5/1996	Weissleder et al.	5,874,109	A 2/1999 Ducheyne et al.
5,527,337	A	6/1996	Stack et al.	5,874,165	A 2/1999 Drumheller
5,545,408	A	8/1996	Trigg et al.	5,876,743	A 3/1999 Ibsen et al.
5,546,646	A *	8/1996	Williams et al. .... 29/407.08	5,877,263	A 3/1999 Patnaik et al.
5,554,120	A	9/1996	Chen et al.	5,879,713	A 3/1999 Roth et al.
5,556,413	A	9/1996	Lam	5,888,533	A 3/1999 Dunn
5,578,046	A	11/1996	Liu et al.	5,891,192	A 4/1999 Murayama et al.
5,578,073	A	11/1996	Haimovich et al.	5,897,955	A 4/1999 Drumheller
5,591,199	A	1/1997	Porter et al.	5,906,759	A 5/1999 Richter
5,591,607	A	1/1997	Gryaznov et al.	5,913,871	A 6/1999 Werneth et al.
5,593,403	A	1/1997	Buscemi	5,914,182	A 6/1999 Drumheller
5,593,434	A	1/1997	Williams	5,916,870	A 6/1999 Lee et al.
5,599,301	A	2/1997	Jacobs et al.	5,922,005	A 7/1999 Richter et al.
				5,942,209	A 8/1999 Leavitt et al.
				5,948,428	A 9/1999 Lee et al.



# US 7,886,419 B2

Page 3

5,954,744 A	9/1999	Phan et al.	6,312,459 B1	11/2001	Huang et al.
5,957,975 A	9/1999	Lafont et al.	6,327,772 B1	12/2001	Zadno-Azizi et al.
5,965,720 A	10/1999	Gryaznov et al.	4,733,665 C2	1/2002	Palmaz
5,971,954 A	10/1999	Conway et al.	6,375,826 B1	4/2002	Wang et al.
5,971,992 A *	10/1999	Solar ..... 606/108	6,379,381 B1	4/2002	Hossainy et al.
5,976,181 A *	11/1999	Whelan et al. .... 623/1.12	6,387,121 B1	5/2002	Alt
5,976,182 A	11/1999	Cox	6,388,043 B1	5/2002	Langer et al.
5,980,564 A	11/1999	Stinson	6,395,326 B1	5/2002	Castro et al.
5,980,928 A	11/1999	Terry	6,409,761 B1	6/2002	Jang
5,980,972 A	11/1999	Ding	6,423,092 B2	7/2002	Datta et al.
5,981,568 A	11/1999	Kunz et al.	6,461,632 B1	10/2002	Gogolewski
5,986,169 A	11/1999	Gjunter	6,464,720 B2	10/2002	Boatman et al.
5,997,468 A	12/1999	Wolff et al.	6,479,565 B1	11/2002	Stanley
6,009,614 A *	1/2000	Morales ..... 29/516	6,485,512 B1	11/2002	Cheng
6,010,445 A	1/2000	Armini et al.	6,492,615 B1	12/2002	Flanagan
6,015,541 A	1/2000	Greff et al.	6,494,908 B1	12/2002	Huxel et al.
6,042,875 A	3/2000	Ding et al.	6,495,156 B2	12/2002	Wenz et al.
6,048,964 A	4/2000	Lee et al.	6,511,748 B1	1/2003	Barrows
6,051,648 A	4/2000	Rhee et al.	6,517,888 B1	2/2003	Weber
6,056,993 A	5/2000	Leidner et al.	6,527,801 B1	3/2003	Dutta
6,060,451 A	5/2000	DiMaio et al.	6,537,589 B1	3/2003	Chae et al.
6,063,092 A *	5/2000	Shin ..... 606/108	6,539,607 B1	4/2003	Fehring et al.
6,066,156 A	5/2000	Yan	6,540,777 B2	4/2003	Stenzel
6,071,266 A	6/2000	Kelley	6,554,854 B1	4/2003	Flanagan
6,074,659 A	6/2000	Kunz et al.	6,565,599 B1	5/2003	Hong
6,080,177 A	6/2000	Igaki et al.	6,569,191 B1	5/2003	Hogan
6,080,488 A	6/2000	Hostettler et al.	6,569,193 B1	5/2003	Cox et al.
6,083,258 A	7/2000	Yadav	6,572,672 B2	6/2003	Yadav et al.
6,093,463 A	7/2000	Thakrar	6,574,851 B1	6/2003	Mirizzi
6,096,070 A	8/2000	Ragheb et al.	6,579,305 B1	6/2003	Lashinski
6,096,525 A	8/2000	Patnaik	6,585,755 B2	7/2003	Jackson et al.
6,099,562 A	8/2000	Ding et al.	6,592,614 B2	7/2003	Lenker et al.
6,103,230 A	8/2000	Billiar et al.	6,592,617 B2	7/2003	Thompson
6,107,416 A	8/2000	Patnaik et al.	6,613,072 B2	9/2003	Lau et al.
6,110,188 A	8/2000	Narciso, Jr.	6,626,939 B1	9/2003	Burnside et al.
6,113,629 A	9/2000	Ken	6,635,269 B1	10/2003	Jennissen
6,117,979 A	9/2000	Hendriks et al.	6,645,243 B2	11/2003	Vallana et al.
6,120,536 A	9/2000	Ding et al.	6,656,162 B2	12/2003	Santini, Jr. et al.
6,120,904 A	9/2000	Hostettler et al.	6,664,335 B2	12/2003	Krishnan
6,121,027 A	9/2000	Clapper et al.	6,666,214 B2	12/2003	Canham
6,125,523 A	10/2000	Brown et al.	6,666,880 B1 *	12/2003	Chiu et al. .... 623/1.11
6,127,173 A	10/2000	Eckstein et al.	6,667,049 B2	12/2003	Janas et al.
6,129,761 A	10/2000	Hubbell	6,669,723 B2	12/2003	Killion et al.
6,129,928 A	10/2000	Sarangapani et al.	6,676,697 B1	1/2004	Richter
6,150,630 A	11/2000	Perry et al.	6,679,980 B1	1/2004	Andreacchi
6,153,252 A	11/2000	Hossainy et al.	6,689,375 B1	2/2004	Wahlig et al.
4,776,337 A	12/2000	Palmaz	6,695,920 B1	2/2004	Pacetti et al.
6,159,951 A	12/2000	Karpeisky et al.	6,706,273 B1	3/2004	Roessler
6,160,084 A	12/2000	Langer et al.	6,709,379 B1	3/2004	Brandau et al.
6,165,212 A	12/2000	Dereume et al.	6,719,934 B2	4/2004	Stinson
6,166,130 A	12/2000	Rhee et al.	6,719,989 B1	4/2004	Matsushima et al.
6,169,170 B1	1/2001	Gryaznov et al.	6,720,402 B2	4/2004	Langer et al.
6,171,609 B1	1/2001	Kunz	6,745,445 B2 *	6/2004	Spilka ..... 29/407.08
6,174,330 B1	1/2001	Stinson	6,746,773 B2	6/2004	Llanos et al.
6,177,523 B1	1/2001	Reich et al.	6,752,826 B2	6/2004	Holloway et al.
6,183,505 B1	2/2001	Mohn, Jr. et al.	6,753,007 B2	6/2004	Haggard et al.
6,187,045 B1	2/2001	Fehring et al.	6,764,505 B1	7/2004	Hossainy et al.
6,210,715 B1	4/2001	Starling et al.	6,769,161 B2 *	8/2004	Brown et al. .... 29/234
6,224,626 B1	5/2001	Steinke	6,818,063 B1	11/2004	Kerrigan
6,228,845 B1	5/2001	Donovan et al.	6,846,323 B2	1/2005	Yip et al.
6,240,616 B1	6/2001	Yan	6,863,683 B2 *	3/2005	Schwager et al. .... 623/1.11
6,245,076 B1	6/2001	Yan	6,958,073 B2 *	10/2005	Rogers et al. .... 606/194
6,245,103 B1	6/2001	Stinson	7,008,446 B1	3/2006	Amis et al.
6,248,344 B1	6/2001	Ylanen et al.	7,563,400 B2 *	7/2009	Wilson et al. .... 264/249
6,251,135 B1	6/2001	Stinson et al.	2001/0044652 A1	11/2001	Moore
6,251,142 B1	6/2001	Bernacca et al.	2002/0002399 A1	1/2002	Huxel et al.
6,273,913 B1	8/2001	Wright et al.	2002/0004060 A1	1/2002	Heublein et al.
6,281,262 B1	8/2001	Shikinami	2002/0004101 A1	1/2002	Ding et al.
6,284,333 B1	9/2001	Wang et al.	2002/0062148 A1	5/2002	Hart
6,287,332 B1	9/2001	Bolz et al.	2002/0065553 A1	5/2002	Weber
6,290,721 B1	9/2001	Heath	2002/0111590 A1	8/2002	Davila et al.
6,293,966 B1	9/2001	Frantzen	2002/0116050 A1	8/2002	Kocur
6,303,901 B1	10/2001	Perry et al.	2002/0138133 A1	9/2002	Lenz et al.



2002/0161114	A1	10/2002	Gunatillake et al.	
2003/0033001	A1	2/2003	Igaki	
2003/0055482	A1	3/2003	Schwager et al.	
2003/0056360	A1	3/2003	Brown et al.	
2003/0093107	A1	5/2003	Parsonage et al.	
2003/0100865	A1	5/2003	Santini, Jr. et al.	
2003/0105518	A1	6/2003	Dutta	
2003/0105530	A1	6/2003	Pirhonen	
2003/0171053	A1	9/2003	Sanders	
2003/0187495	A1	10/2003	Cully et al.	
2003/0208259	A1	11/2003	Penhasi	
2003/0209835	A1	11/2003	Chun et al.	
2003/0226833	A1	12/2003	Shapovalov et al.	
2003/0236563	A1	12/2003	Fifer	
2004/0078953	A1	4/2004	Spilka	
2004/0093077	A1	5/2004	White et al.	
2004/0098095	A1	5/2004	Burnside et al.	
2004/0111149	A1	6/2004	Stinson	
2004/0127970	A1	7/2004	Weber	
2004/0143317	A1	7/2004	Stinson et al.	
2004/0167610	A1	8/2004	Fleming, III	
2005/0143752	A1 *	6/2005	Schwager et al. ....	606/108
2006/0009832	A1 *	1/2006	Fisher .....	623/1.11
2006/0047336	A1	3/2006	Gale et al.	
2006/0142834	A1 *	6/2006	Rizq et al. ....	623/1.11
2006/0288561	A1 *	12/2006	Roach et al. ....	29/508
2007/0006441	A1 *	1/2007	McNiven et al. ....	29/508
2007/0129786	A1 *	6/2007	Beach et al. ....	623/1.15
2007/0204455	A1 *	9/2007	Knott et al. ....	29/508
2007/0289117	A1 *	12/2007	Huang et al. ....	29/508
2008/0001328	A1 *	1/2008	Kent et al. ....	264/268
2008/0028594	A1 *	2/2008	Lafont et al. ....	29/516
2009/0088829	A1 *	4/2009	Wang et al. ....	623/1.11
2009/0208552	A1 *	8/2009	Faucher et al. ....	424/423
2009/0259289	A1 *	10/2009	Wilson et al. ....	623/1.11
2010/0063571	A1 *	3/2010	Roach et al. ....	623/1.11

## FOREIGN PATENT DOCUMENTS

DE	197 31 021	1/1999
DE	198 56 983	12/1999
EP	0 108 171	5/1984
EP	0 144 534	6/1985
EP	0 364 787	4/1990
EP	0 397 500	11/1990
EP	0 464 755	1/1992
EP	0 493 788	7/1992
EP	0 554 082	8/1993
EP	0 578 998	1/1994
EP	0 604 022	6/1994
EP	0 621 017	10/1994
EP	0 623 354	11/1994
EP	0 665 023	8/1995
EP	0 709 068	5/1996
EP	0 970 711	1/2000
EP	1295570	A2 * 3/2003
GB	2 247 696	3/1992
WO	WO 89/03232	4/1989
WO	WO 90/01969	3/1990
WO	WO 90/04982	5/1990
WO	WO 90/06094	6/1990
WO	WO 91/17744	11/1991
WO	WO 91/17789	11/1991
WO	WO 92/10218	6/1992
WO	WO 93/06792	4/1993
WO	WO 94/21196	9/1994
WO	WO 95/29647	11/1995
WO	WO 98/04415	2/1998
WO	WO 99/03515	1/1999
WO	WO 99/15106	4/1999
WO	WO 99/16386	4/1999
WO	WO 99/42147	8/1999
WO	WO 00/12147	3/2000

WO	WO 00/64506	11/2000
WO	WO 01/01890	1/2001
WO	WO 02/30487	4/2002
WO	WO 2004/023985	3/2004

## OTHER PUBLICATIONS

U.S. Appl. No. 10/317,435, filed Dec. 11, 2002, Hossainy et al.

Anonymous, *Bioabsorbable stent mounted on a catheter having optical coherence tomography capabilities*, Research Disclosure, Sep. 2004, pp. 1159-1162.

Ansari, *End-to-end tubal anastomosis using an absorbable stent*, Fertility and Sterility, vol. 32(2), pp. 197-201 (Aug. 1979).

Ansari, *Tubal Reanastomosis Using Absorbable Stent*, International Journal of Fertility, vol. 23(4), pp. 242-243 (1978).

Bull, *Parylene Coating for Medical Applications*, Medical Product Manufacturing News 18, 1 pg. (Mar. 1993).

Casper et al., *Fiber-Reinforced Absorbable Composite for Orthopedic Surgery*, Polymeric Materials Science and Engineering, vol. 53 pp. 497-501 (1985).

Detweiler et al., *Gastrointestinal Sutureless Anastomosis Using Fibrin Glue: Reinforcement of the Sliding Absorbable Intraluminal Nontoxic Stent and Development of a Stent Placement Device*, Journal of Investigative Surgery, vol. 9(2), pp. 111-130 (Mar./Apr. 1996).

Detweiler et al., *Sliding, Absorbable, Reinforced Ring and an Axially Driven Stent Placement Device for Sutureless Fibrin Glue Gastrointestinal Anastomosis*, Journal of Investigative Surgery, vol. 9(6), pp. 495-504 (Nov./Dec. 1996).

Detweiler et al., *Sutureless Anastomosis of the Small Intestine and the Colon in Pigs Using an Absorbable Intraluminal Stent and Fibrin Glue*, Journal of Investigative Surgery, vol. 8(2), pp. 129-140 (Mar. 1995).

Detweiler et al., *Sutureless Cholecystojejunostomy in Pigs Using an Absorbable Intraluminal Stent and Fibrin Glue*, Journal of Investigative Surgery, vol. 9(1), pp. 13-26 (Jan./Feb. 1996).

Devanathan et al., *Polymeric Conformal Coatings for Implantable Electronic Devices*, IEEE Transactions on Biomedical Engineering, vol. BME-27(11), pp. 671-675 (1980).

Elbert et al., *Conjugate Addition Reactions Combined with Free-Radical Cross-Linking for the Design of Materials for Tissue Engineering*, Biomacromolecules, vol. 2, pp. 430-441 (2001).

Hahn et al., *Biocompatibility of Glow-Discharge-Polymerized Films and Vacuum-Deposited Parylene*, J Applied Polymer Sci, vol. 38, pp. 55-64 (1984).

Hahn et al., *Glow Discharge Polymers as Coatings for Implanted Devices*, ISA, pp. 109-111 (1981).

He et al., *Assessment of Tissue Blood Flow Following Small Artery Welding with an Intraluminal Dissolvable Stent*, Microsurgery, vol. 19(3), pp. 148-152 (1999).

Kelley et al., *Totally Resorbable High-Strength Composite Material*, Advances in Biomedical Polymers, vol. 35, pp. 75-85 (1987).

Kubies et al., *Microdomain Structure In polylactide-block-poly(ethylene oxide) copolymer films*, Biomaterials, vol. 21, pp. 529-536 (2000).

Kutryk et al., *Coronary Stenting: Current Perspectives*, a companion to the Handbook of Coronary Stents, pp. 1-16 (1999).

Martin et al., *Enhancing the biological activity of immobilized osteopontin using a type-1 collagen affinity coating*, J. Biomed. Mater. Res., vol. 70A, pp. 10-19 (2004).

Mauduit et al., *Hydrolytic degradation of films prepared from blends of high and low molecular weight poly(DL-lactic acid)s*, J. Biomed. Mater. Res., vol. 30, pp. 201-207 (1996).

Middleton et al., *Synthetic biodegradable polymers as orthopedic devices*, Biomaterials, vol. 21, pp. 2335-2346 (2000).

Muller et al., *Advances in Coronary Angioplasty: Endovascular Stents*, Coron. Arter. Dis., vol. 1(4), pp. 438-448 (Jul./Aug. 1990).

Nichols et al., *Electrical Insulation of Implantable Devices by Composite Polymer Coatings*, ISA Transactions, vol. 26(4), pp. 15-18 (1987).

Peuster et al., *A novel approach to temporary stenting: degradable cardiovascular stents produced from corrodible metal—results 6-18 months after implantation into New Zealand white rabbits*, Heart, vol. 86, pp. 563-569 (2001).

Pietrzak et al., *Bioabsorbable Fixation Devices: Status for the Craniomaxillofacial Surgeon*, J. Craniofacial Surg., vol. 2, pp. 92-96 (1997).

Pietrzak et al., *Bioresorbable implants—practical considerations*, Bone, vol. 19, No. 1, Supplement Jul. 1996, pp. 109S-119S.

Redman, *Clinical Experience with Vasovasostomy Utilizing Absorbable Intravasal Stent*, Urology, vol. 20(1), pp. 59-61 (Jul. 1982).

Rust et al., *The Effect of Absorbable Stenting on Postoperative Stenosis of the Surgically Enlarged Maxillary Sinus Ostia in a Rabbit Animal Model*, Archives of Otolaryngology, vol. 122(12) pp. 1395-1397 (Dec. 1996).

Schatz, *A View of Vascular Stents*, Circulation, vol. 79(2), pp. 445-457 (Feb. 1989).

Schmidt et al., *Long-Term Implants of Parylene-C Coated Microelectrodes*, Med & Biol Eng & Comp, vol. 26(1), pp. 96-101 (Jan. 1988).

Spagnuolo et al., *Gas 1 is induced by VE-cadherin and vascular endothelial growth factor and inhibits endothelial cell apoptosis*, Blood, vol. 103, pp. 3005-3012 (2004).

Tamai et al., *Initial and 6-Month Results of Biodegradable Poly-L-Lactic Acid Coronary Stents in Humans*, Circulation, pp. 399-404 (Jul. 25, 2000).

Tsuji et al., *Biodegradable Polymeric Stents*, Current Interventional Cardiology Reports, vol. 3, pp. 10-17 (2001).

Völkel et al., *Targeting of immunoliposomes to endothelial cells using a single-chain Fv fragment directed against human endoglin (CD105)*, Biochimica et Biophysica Acta 1663, pp. 158-166 (2004).

von Recum et al., *Degradation of polydispersed poly(L-lactic acid) to modulate lactic acid release*, Biomaterials, vol. 16, pp. 441-445 (1995).

Yau et al., *Modern Size-Exclusion Liquid Chromatography*, Wiley-Interscience Publication, IX-XV (1979).

International Search Report for PCT/US2007/014331 filed Jun. 19, 2007, mailed Dec. 28, 2007, 13 pgs.

\* cited by examiner



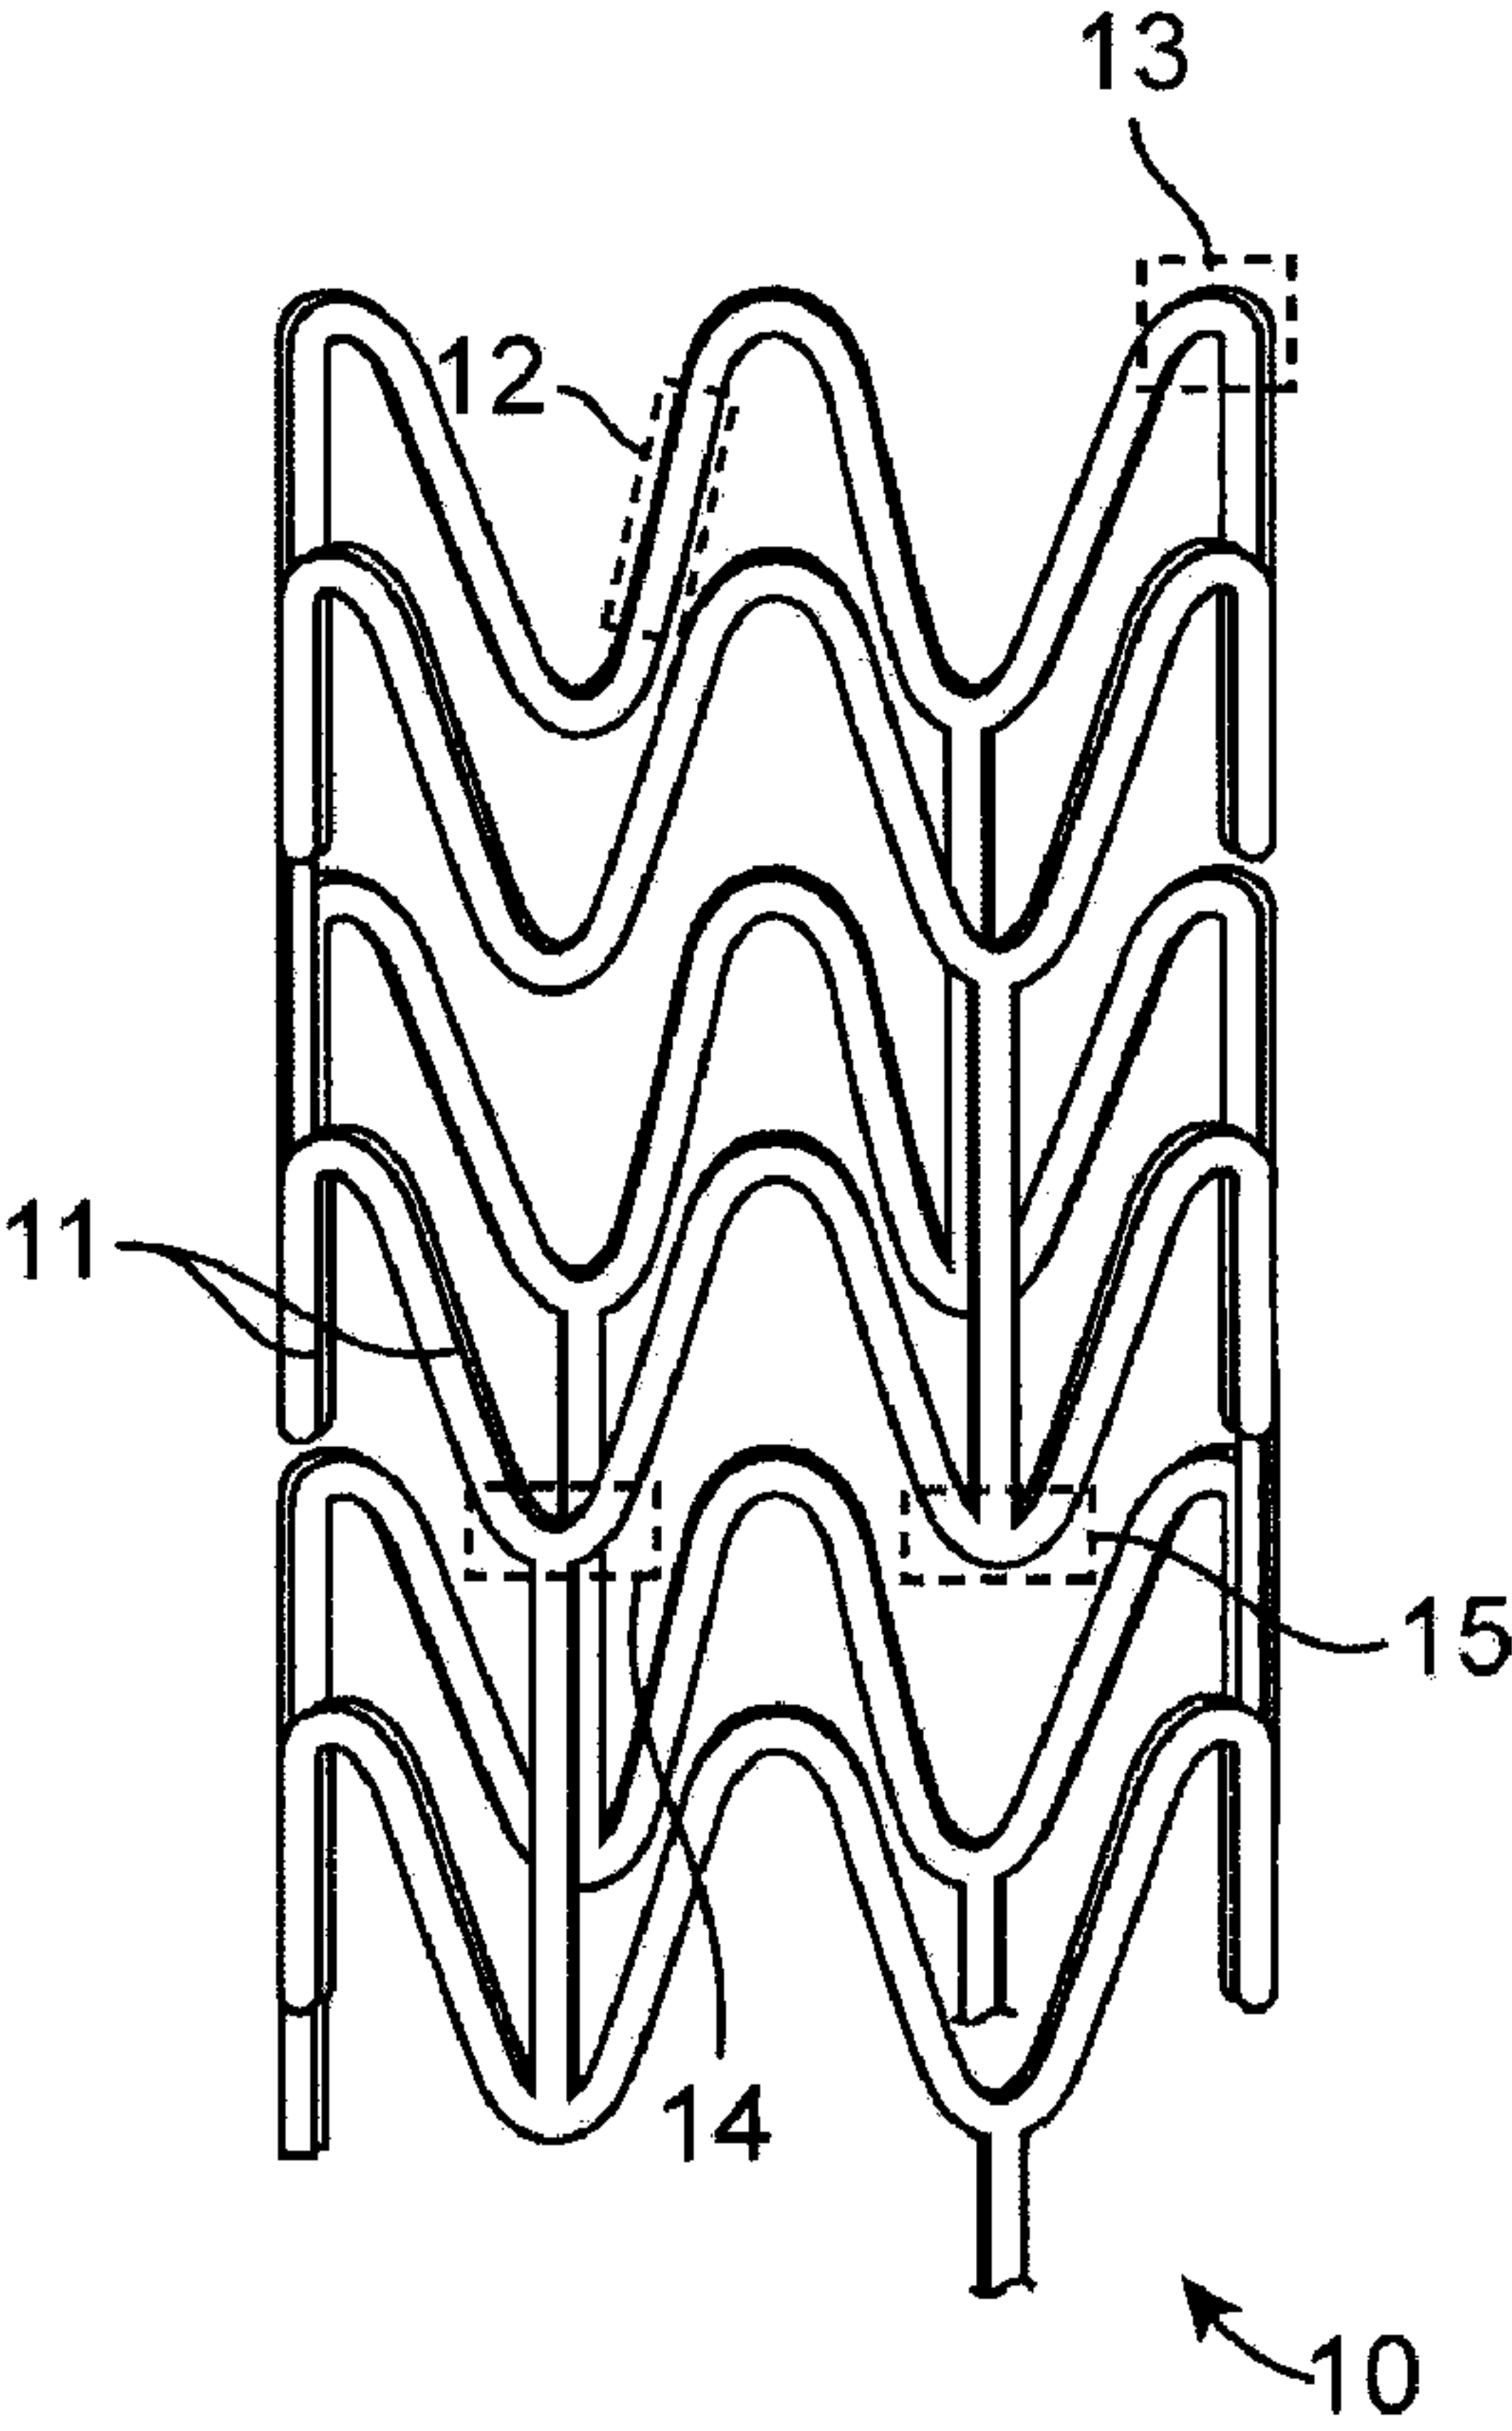


FIG. 1

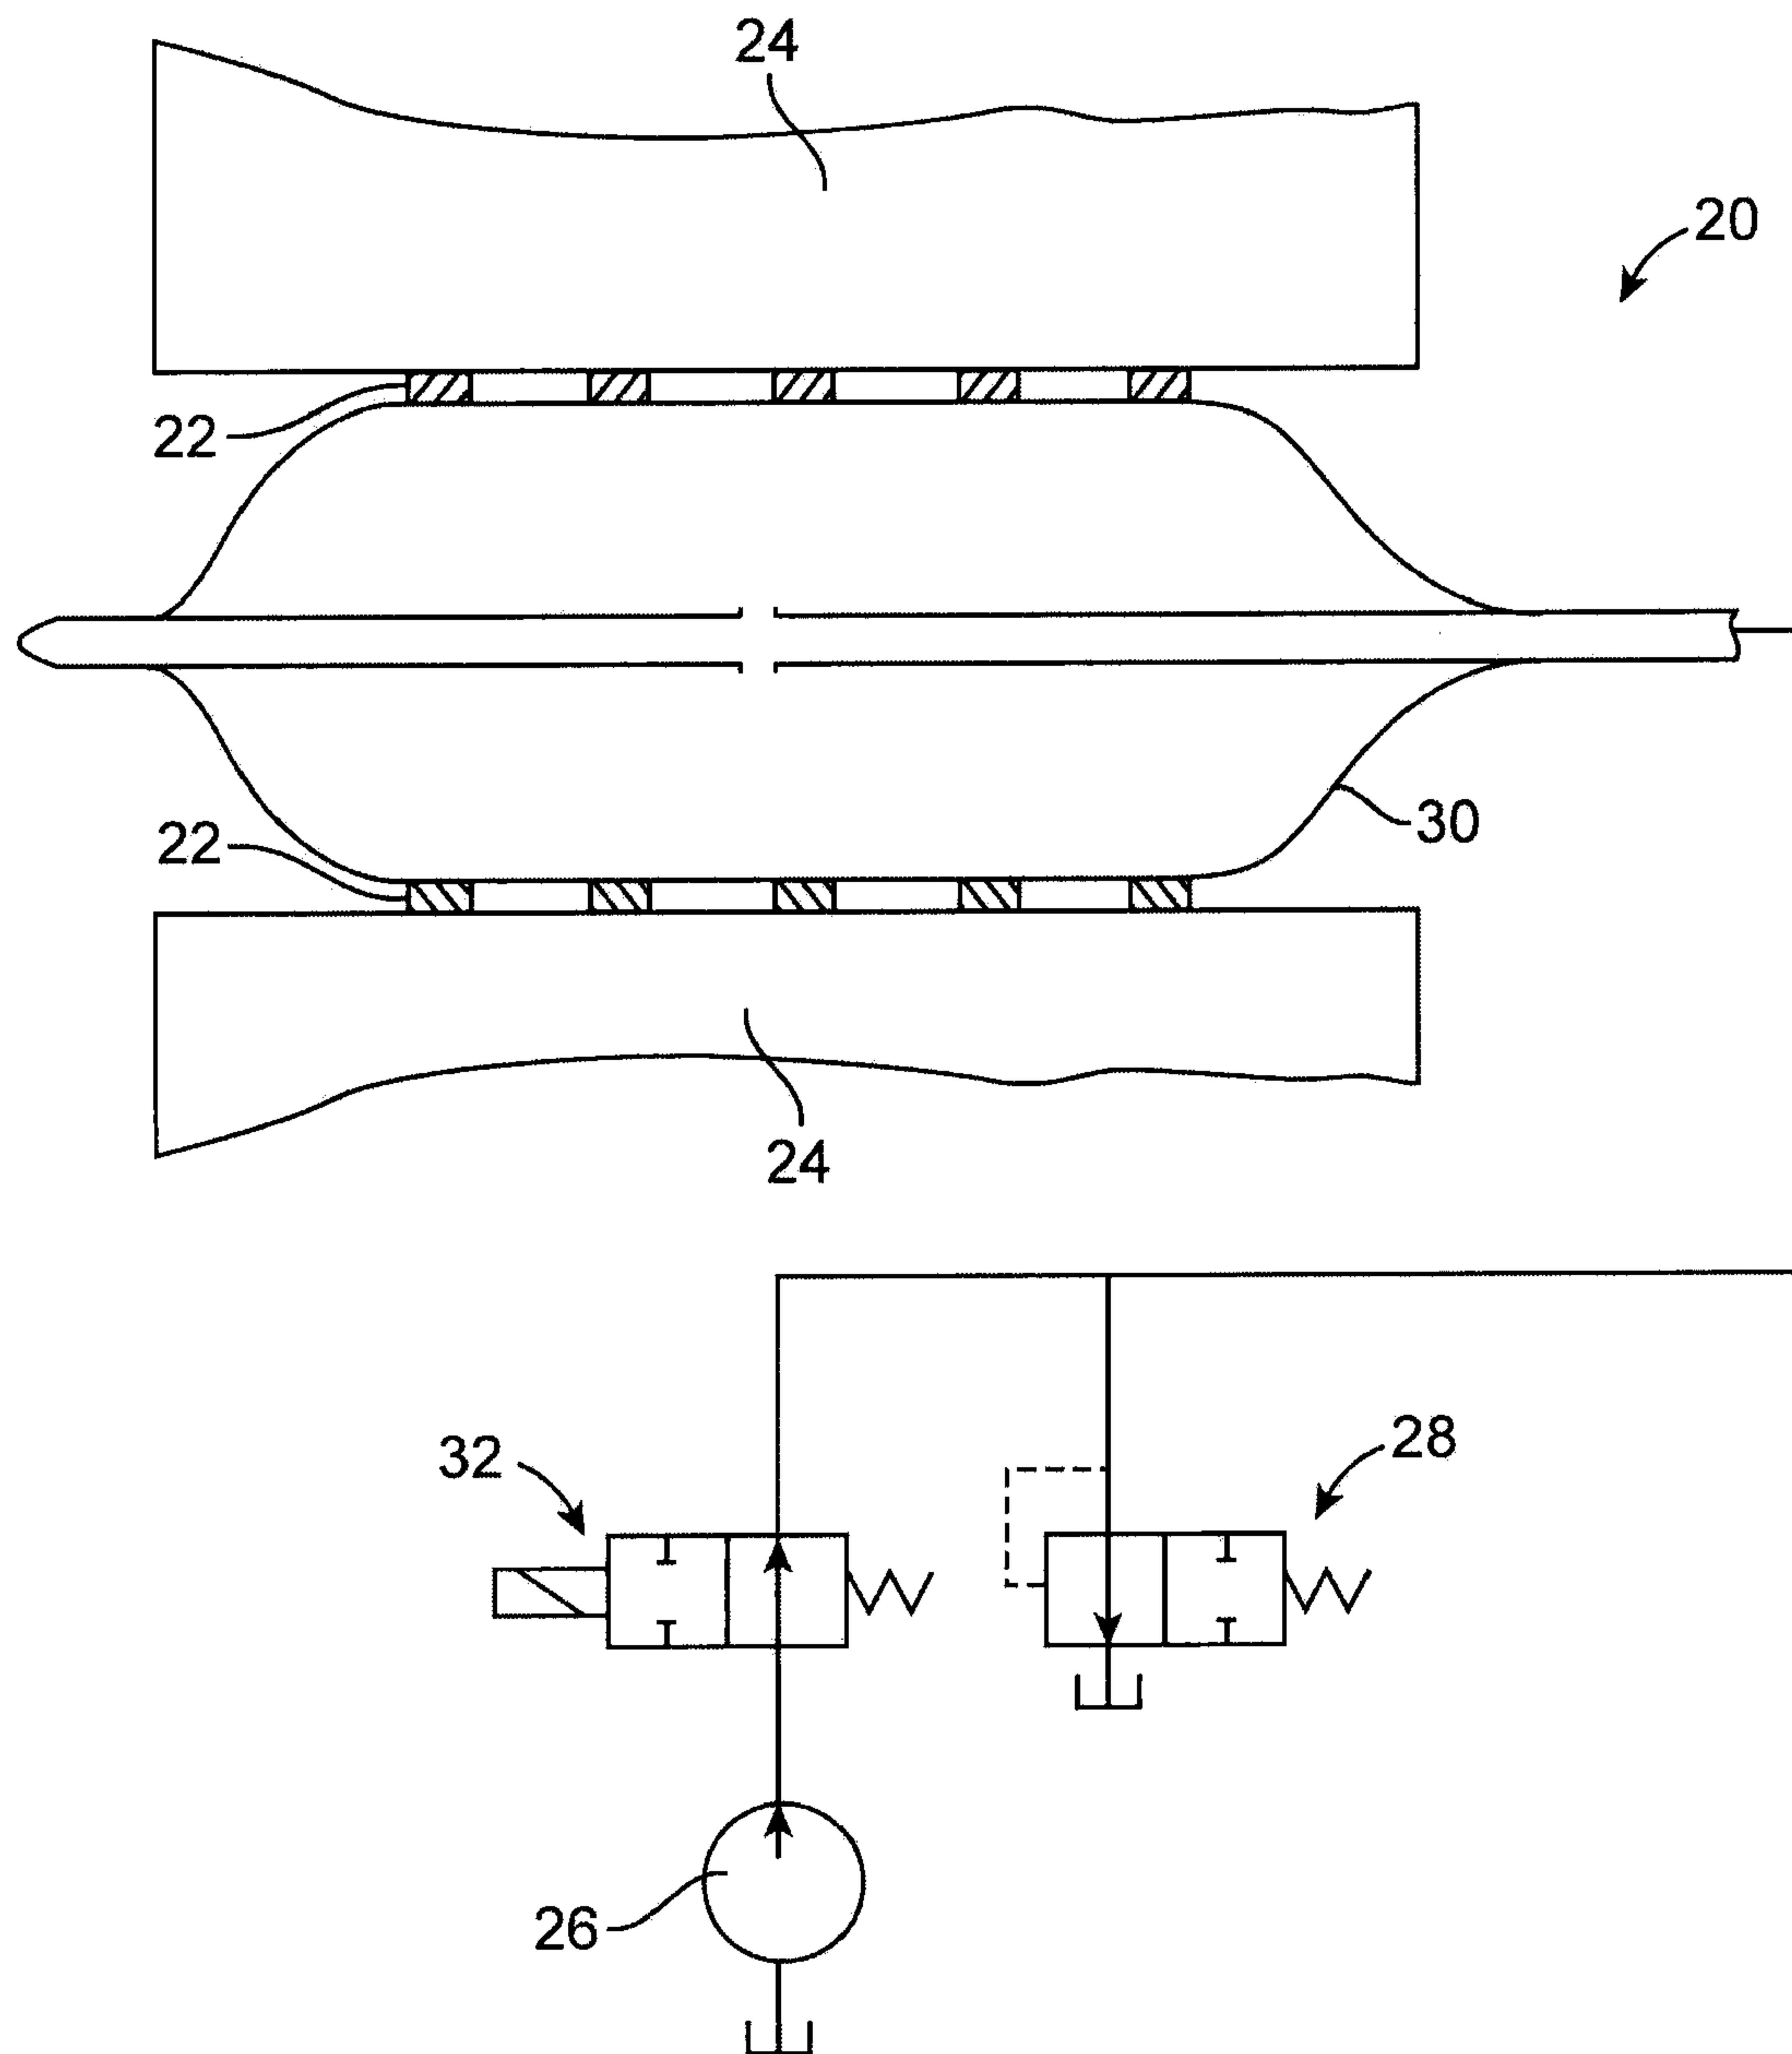


FIG. 2

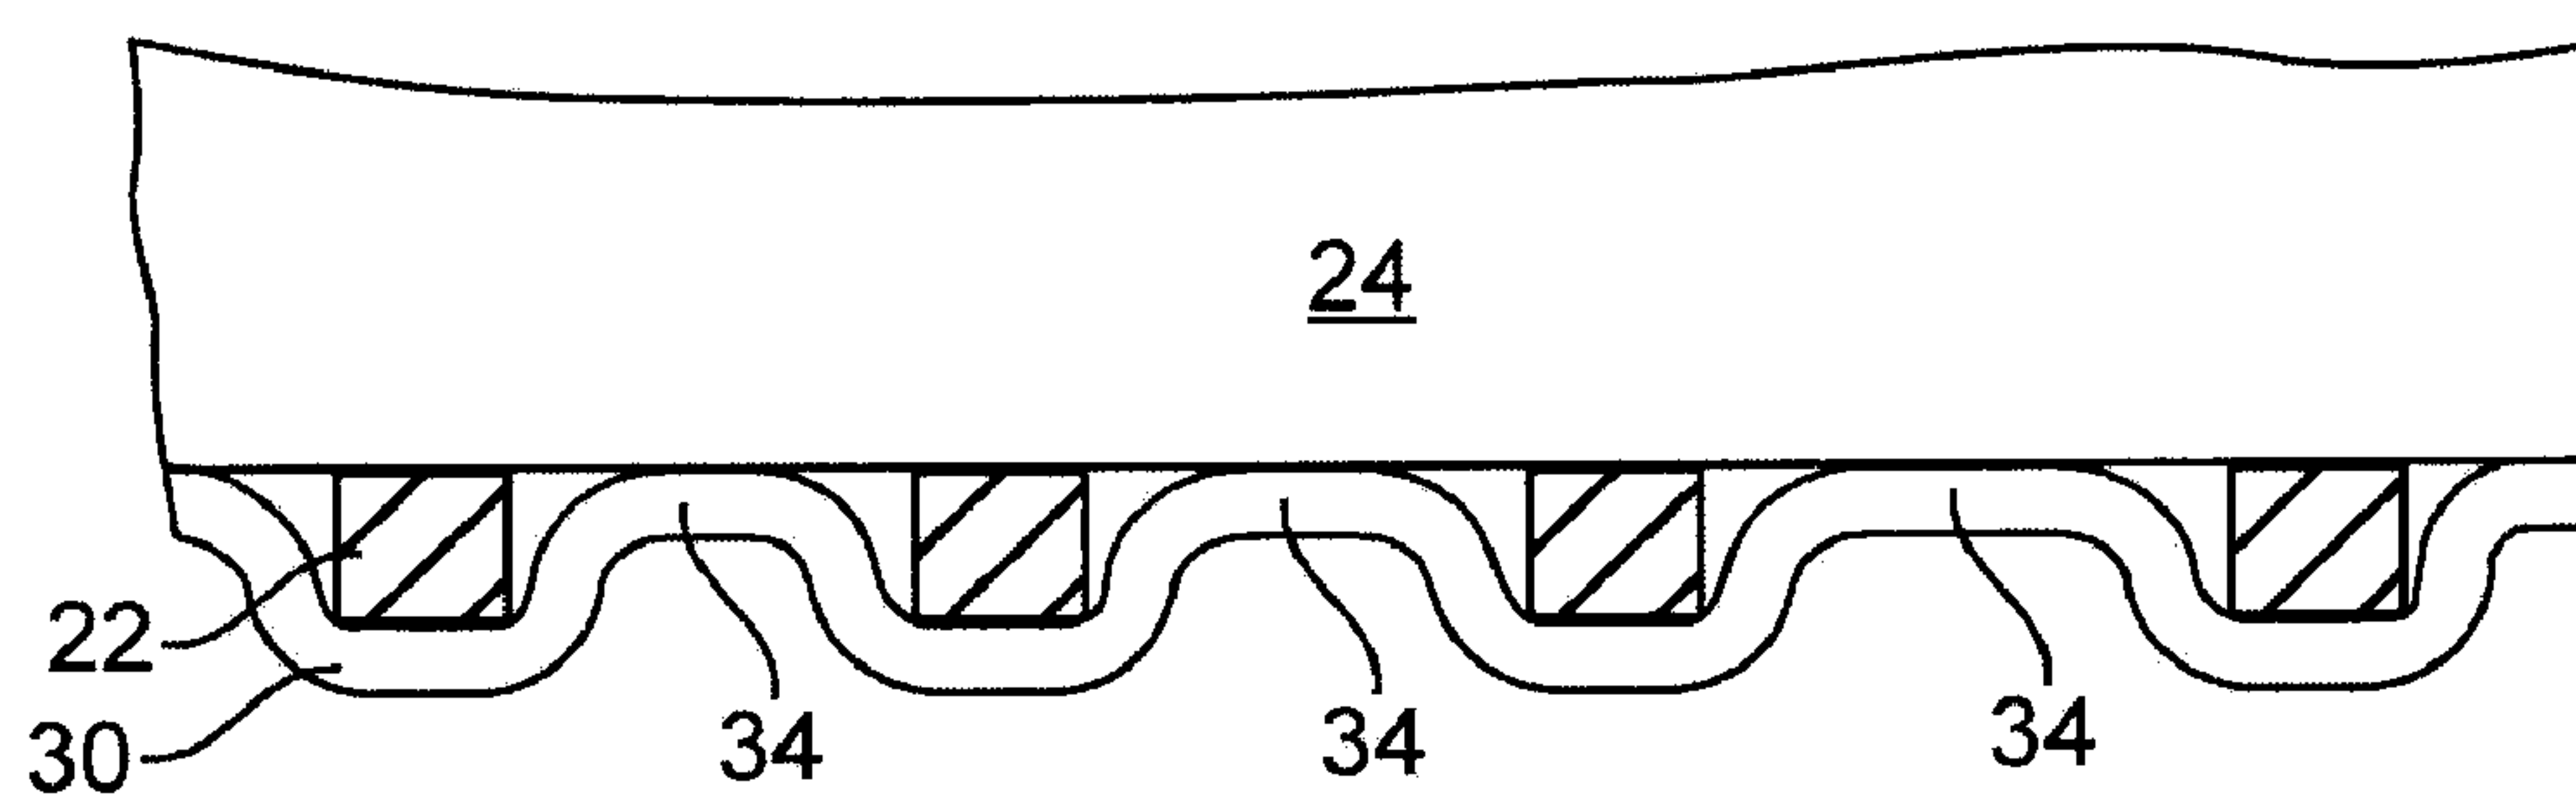


FIG. 3



## 1

**STENT CRIMPING APPARATUS AND  
METHOD**

## FIELD OF THE INVENTION

This invention relates to an apparatus for crimping a stent and a method for crimping a stent.

## BACKGROUND

A typical stent is a cylindrically shaped device, which holds open and sometimes expands a segment of a blood vessel or other anatomical lumen such as urinary tracts and bile ducts. Stents are often used in the treatment of atherosclerotic stenosis in blood vessels. "Stenosis" refers to a narrowing or constriction of the diameter of a bodily passage or orifice. In such treatments, stents reinforce body vessels and prevent restenosis following angioplasty. "Restenosis" refers to the reoccurrence of stenosis in a blood vessel or heart valve after it has been subjected to angioplasty or valvuloplasty.

A stent is typically composed of scaffolding that includes a pattern or network of interconnecting structural elements often referred to in the art as struts or bar arms. The scaffolding can be formed from wires, tubes, or sheets of material rolled into a cylindrical shape.

In the case of a balloon expandable stent, the stent is mounted on a balloon connected to a catheter. A typical conventional method of mounting the stent on the balloon is a two-step process. First, the stent is compressed or crimped onto the balloon. Second, the compressed or crimped stent is retained or secured on the balloon. The retained stent should have a sufficiently small diameter so that it can be transported through the narrow passages of blood vessels. The stent must be secured on the balloon during delivery until it is deployed at an implant or treatment site within a vessel in the body of a patient. The stent is then expanded by inflating the balloon. "Delivery" refers to introducing and transporting the crimped stent through a bodily lumen to the treatment site in a vessel. "Deployment" corresponds to the expanding of the crimped stent within the lumen at the treatment site. Delivery and deployment of a stent are accomplished by positioning the stent about one end of a catheter, inserting the end of the catheter through the skin into a bodily lumen, advancing the catheter in the bodily lumen to a desired treatment location, inflating the stent at the treatment location, and removing the catheter from the lumen by deflating the balloon.

The stent should be firmly secured to the balloon to avoid detachment of the stent before it is delivered and deployed in the lumen of the patient. Detachment of a stent from the balloon during delivery and deployment can result in medical complications. A lost stent can act as an embolus that can create a thrombosis and require surgical intervention. For this reason, a stent must be securely attached to the catheter. Stent retention is greatly enhanced by protrusion of the balloon into the interstitial spaces or gaps between stent struts.

Stent retention for a polymer stent is especially challenging. Because polymers generally have lower strength than metals, a polymer stent requires wider struts than a metal stent to achieve the same mechanical strength. As a result, a polymer stent has smaller spaces or gaps between adjacent struts, making it more difficult for a balloon to protrude into the spaces to enhance stent retention. Additionally, a polymer stent may have a similar  $T_g$  as the balloon material so that there is a limitation on the use of high temperature to enhance balloon protrusion into stent gaps. When high temperature is

## 2

used during a crimping process, the stent tends to return to its original dimension and lose its preferred mechanical properties.

## SUMMARY

The present invention overcomes the above disadvantage of the prior art. In an preferred embodiment of the present invention, the balloon may be inflated when the stent is crimped onto the balloon, allowing the balloon to extend into the gaps of the stent to enhance stent retention.

In accordance with one aspect of the invention, a method for crimping a stent onto a balloon includes inflating a balloon with a fluid such as a gas or a liquid, sliding a stent over the inflated balloon, crimping the stent onto the balloon, and controlling the pressure inside the balloon below a given value when the stent is being crimped onto the balloon.

In a preferred embodiment of the invention, the step of controlling includes releasing the fluid inside the balloon when the pressure exceeds the given value so that the pressure inside the balloon does not exceed the given value.

In another preferred embodiment of the invention, the step of releasing includes using a pressure release valve to control the fluid inside the balloon below the given value.

In still another preferred embodiment of the invention, the method includes placing the stent and balloon in a crimper before the stent is crimped onto the balloon.

In a further embodiment of the invention, the method includes soaking the balloon in a solvent to soften the balloon. The solvent may be acetone.

In accordance with another aspect of the invention, a method for crimping a stent onto a balloon includes sliding a stent over a balloon, placing the stent and balloon in a stent crimper, inflating the balloon with a fluid such as a gas or a liquid, crimping the stent onto the balloon, and controlling the pressure inside the balloon below a given value when the stent is being crimped onto the balloon.

In a preferred embodiment of the invention, the method includes reducing the crimper's inner diameter to the outer diameter of the stent before inflating the balloon with the fluid.

In another preferred embodiment of the invention, the step of controlling includes releasing the fluid inside the balloon when the pressure exceeds the given value so that the pressure inside the balloon does not exceed the given value.

In still another preferred embodiment of the invention, the step of releasing includes using a pressure release valve to control the fluid inside the balloon below the given value.

In a further embodiment of the invention, the method includes soaking the balloon in a solvent to soften the balloon. The solvent may be acetone.

In accordance with a further aspect of the invention, a stent crimping apparatus includes means for inflating a balloon with a fluid such as a gas or a liquid, means for crimping the stent onto the balloon, and means for controlling the pressure inside the balloon below a given value when the stent is being crimped onto the balloon.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a perspective view of a stent.

FIG. 2 shows one apparatus for crimping a stent according to the present invention.

FIG. 3 shows portions of a balloon extending into the gaps of a stent.



## DETAILED DESCRIPTION OF THE INVENTION

Those of ordinary skill in the art will realize that the following description of the invention is illustrative only and not in any way limiting. Other embodiments of the invention will readily suggest themselves to such skilled persons based on the disclosure herein. All such embodiments are within the scope of this invention.

FIG. 1 illustrates a stent **10** that includes a number of interconnecting structural elements or struts **11**. In general, the pattern of the stent struts is designed so that the stent can be radially compressed and expanded. The stent may include portions of struts that are straight or relatively straight, an example being a straight portion designated by reference numeral **12**. The stent may also include portions of struts that are bent, such as the portions designated by reference numerals **13**, **14**, and **15**. The bent portions **13**, **14**, and **15** may bend further when the stent **10** is crimped radially inwardly. The bent portions **13**, **14**, and **15** may bend less when the stent **10** is expanded radially outwardly.

A stent, as fabricated, is uncrimped and may have an outside diameter that is typically from about 1 mm and to about 4 mm. When the stent is crimped, the structural elements deform allowing the stent to decrease in diameter. The deformation occurs primarily at the bending elements. The balloon, when mounted on a catheter, may have an outside diameter of between about 0.7 mm and 0.8 mm. The outside diameter of a crimped stent may be approximately the same as the outside diameter of the balloon.

In some embodiments, a stent of the present invention may be formed from a tube by laser cutting the pattern of structural elements in the tube. The stent may also be formed by laser cutting a polymeric or metallic sheet, rolling the pattern into the shape of the cylindrical stent, and providing a longitudinal weld to form the stent. Other methods of forming stents are well known and include chemically etching a polymeric or metallic sheet and rolling and then welding it to form the stent. A polymeric or metallic wire may also be coiled to form the stent. The stent may be formed by injection molding of a thermoplastic or reaction injection molding of a thermoset polymeric material. Filaments of the compounded polymer may be extruded or melt spun. These filaments can then be cut, formed into ring elements, welded closed, corrugated to form crowns, and then the crowns welded together by heat or solvent to form the stent. Lastly, hoops or rings may be cut from tubing stock, the tube elements stamped to form crowns, and the crowns connected by welding or laser fusion to form the stent.

A stent can be made from one or more suitable materials. For example, a stent may be made from a metallic material. Alternatively, a stent may be made from a polymeric material. A stent may include a biodegradable material, such as a biodegradable polymer or metal. The biodegradable material may be a pure or substantially pure biodegradable polymer or metal. Alternatively, the biodegradable material may be a mixture of at least two types of biodegradable polymers and metals.

Representative examples of polymers that may be used to fabricate embodiments of stents, or more generally, implantable medical devices include, but are not limited to, poly(N-acetylglucosamine) (Chitin), Chitosan, poly(3-hydroxyvalerate), poly(lactide-co-glycolide), poly(3-hydroxybutyrate), poly(4-hydroxybutyrate), poly(3-hydroxybutyrate-co-3-hydroxyvalerate), polyorthoester, polyanhydride, poly(glycolic acid), poly(glycolide), poly(L-lactic acid), poly(L-lactide), poly(D,L-lactic acid), poly(D,L-lactide), poly(L-lactide-co-D,L-lactide), poly(caprolactone), poly(L-lactide-co-capro-

lactone), poly(D,L-lactide-co-caprolactone), poly(glycolide-co-caprolactone), poly(trimethylene carbonate), polyester amide, poly(glycolic acid-co-trimethylene carbonate), co-poly(ether-esters) (e.g. PEO/PLA), polyphosphazenes, biomolecules (such as fibrin, fibrinogen, cellulose, starch, collagen, and hyaluronic acid), polyurethanes, silicones, polyesters, polyolefins, polyisobutylene and ethylene-alpha-olefin copolymers, acrylic polymers and copolymers, vinyl halide polymers and copolymers (such as polyvinyl chloride), polyvinyl ethers (such as polyvinyl methyl ether), polyvinylidene halides (such as polyvinylidene chloride), polyacrylonitrile, polyvinyl ketones, polyvinyl aromatics (such as polystyrene), polyvinyl esters (such as polyvinyl acetate), acrylonitrile-styrene copolymers, ABS resins, polyamides (such as Nylon 66 and polycaprolactam), polycarbonates, polyoxymethylenes, polyimides, polyethers, polyurethanes, rayon, rayon-triacetate, cellulose acetate, cellulose butyrate, cellulose acetate butyrate, cellophane, cellulose nitrate, cellulose propionate, cellulose ethers, and carboxymethyl cellulose. Additional representative examples of polymers that may be especially well suited for use in fabricating embodiments of implantable medical devices disclosed herein include ethylene vinyl alcohol copolymer (commonly known by the generic name EVOH or by the trade name EVAL), poly(butyl methacrylate), poly(vinylidene fluoride-co-hexafluoropropene) (e.g., SOLEF 21508, available from Solvay Solexis PVDF, Thorofare, N.J.), polyvinylidene fluoride (otherwise known as KYNAR, available from ATOFINA Chemicals, Philadelphia, Pa.), ethylene-vinyl acetate copolymers, poly(vinyl acetate), styrene-isobutylene-styrene triblock copolymers, and polyethylene glycol.

FIG. 2 illustrates one apparatus **20** for crimping a stent **22** according to the present invention. In the present invention, to "crimp" a stent is to compress the stent radially inward to reduce its diameter. The apparatus **20** may include one or more crimping elements **24**, a source **26** for pressurized fluid, and a pressure control device **28**.

The crimping elements **24** can be used to crimp the stent **22**. The crimping elements **24** may be any of the known crimping devices that can move radially to crimp the stent **22**. Such crimping elements (or device) are well known in the art and will not be described in detail here.

The pressurized fluid source **26** can be used to supply pressurized fluid, such as pressurized gas or liquid, to inflate a balloon **30**, on which the stent **22** is mounted. The balloon **28** may be part of a catheter (not shown). The pressurized fluid source **26** may be any device that can supply pressurized fluid, such as a pump or an accumulator. In the illustrated embodiment, the pressurized fluid source **26** is a pump **26**. Preferably, a valve **32** is provided that can shut off the pressurized fluid supplied by the pump **26** to the balloon **30**.

The pressure control device **28** may be used to control the pressure inside the balloon **30**. For example, the pressure control device **28** may keep the pressure inside of the balloon **30** below a predetermined value. The pressure control device may be any suitable device for achieving this purpose. In the illustrated embodiment, the pressure control device **28** is a pressure relief valve **28**.

To crimp the stent **22** on the balloon **30** in accordance with one method of the present invention, the balloon **30** is first inflated using the pressurized fluid supplied by the pump **26** (or any other suitable pressurized fluid source). To soften the balloon **30**, the balloon **30** may be soaked in a solvent, such as acetone, for a predetermine period of time. After the stent **22** at a first diameter value has been slid on the inflated balloon **30**, the stent **22** and balloon **30** are placed in the stent crimping apparatus **20**. Next, the crimping elements **24** may radially



## 5

compress the stent **22** to reduce the stent's diameter to a second diameter value while the balloon remains inflated. During crimping, the balloon pressure may be kept at or below a first pressure value by the pressure relief valve **28**. If the pressure inside the balloon **30** is above the first pressure value, the pressure relief valve **28** opens to discharge the pressurized fluid inside the balloon until the pressure reaches or is below the first pressure value. After the diameter of the stent has been reduced to the second diameter value, the balloon pressure may be kept at the first pressure value for a first period of time. Then the pressure inside the balloon may be released for a second period of time. Next the balloon is inflated again to a second pressure value, and the stent is crimped again until its diameter reaches a third diameter value. The balloon pressure may be kept at the second pressure value for a third period of time. Then the pressure inside the balloon may be released, and the stent and balloon may be removed from the stent crimping apparatus **20**.

To crimp the stent **22** on the balloon **30** in accordance with another method of the present invention, the stent **22** is first slid on the balloon **30** without the balloon **30** being inflated. To soften the balloon **30**, the balloon **30** may be soaked in a solvent, such as acetone, for a predetermine period of time. Then the stent **22** and balloon **30** are placed in the stent crimping apparatus **20**. Next the stent **22** may be radially compressed from a first diameter value to a second diameter value while the balloon is not inflated. After the diameter of the stent has been reduced to the second diameter value, the balloon may be inflated to a first pressure value for a first period of time. Then the stent is crimped again until its diameter reaches a third diameter value. The balloon pressure may be kept at the first pressure value for a second period of time. Then the pressure inside the balloon may be released, and the stent and balloon may be removed from the stent crimping apparatus **20**.

FIG. **3** shows that after the stent **22** has been crimped onto the balloon **30** using a method of the present invention, portions **34** of the balloon **30** extend into the gaps of the stent **22**.

The following are two examples of stent crimping using a method of the present invention.

## Example I

The outer diameter of a pre-crimp stent is 0.135 inches. The balloon is inflated to 39 psi, and the stent is mounted on the balloon. The stent and balloon are placed in a stent crimping apparatus, and the stent is crimped to 0.090 inches while the balloon pressure is kept at 39 psi. Next, the balloon pressure is kept at 39 psi for 20 seconds. Afterwards, the balloon may be deflated for a period of time. The crimper then reduces the outer diameter of the stent to 0.045 inches for 50 seconds without balloon pressure. The balloon is inflated again for 20 seconds under 39 psi. Then the balloon pressure is reduced to zero for 20 seconds. Finally, the stent and balloon are removed from the crimper.

## Example II

The outer diameter of an uncrimped stent is 0.084 inches. The uncrimped stent is placed in a crimper, and the crimper's inner diameter is reduced to 0.084 inches, which is the outer diameter of the uncrimped stent. Next, the balloon is inflated under 30 psi pressure for 20 seconds. The crimper then reduces the outer diameter of the stent to 0.032 inches under 30 psi for five seconds and then for 45 seconds without balloon pressure. The balloon is inflated again for 25 seconds

## 6

under 30 psi. Then the balloon pressure is reduced to zero for 10 seconds. Finally, the stent and balloon are removed from the crimper.

While particular embodiments of the present invention have been shown and described, it will be obvious to those skilled in the art that changes and modifications can be made without departing from this invention in its broader aspects.

What is claimed is:

**1.** A method for crimping a stent onto a balloon, comprising:

inflating a balloon with a fluid to a first pressure value;  
sliding a stent at a first diameter over the inflated balloon;  
crimping the stent to a second diameter that is less than the first diameter onto the balloon;

after crimping the stent to the second diameter, releasing the pressure from inside the balloon so that the balloon is deflated;

inflating the balloon that is deflated to a second pressure value;

crimping the stent to a third diameter that is less than the second diameter after inflating the balloon to the second pressure value; and

controlling the pressure inside the balloon below the first pressure value when crimping to the second diameter and below the second pressure value when crimping to the third diameter.

**2.** The method of claim **1**, wherein the step of controlling includes releasing the fluid inside the balloon when the pressure exceeds the first pressure value or second pressure value so that the pressure inside the balloon does not exceed the first pressure value or second pressure value, respectively.

**3.** The method of claim **2**, wherein the step of releasing includes using a pressure release valve to control the fluid inside the balloon below the first or second pressure value.

**4.** The method of claim **1**, further comprising placing the stent and balloon in a crimper before the stent is crimped to the second diameter onto the balloon.

**5.** The method of claim **1**, further comprising soaking the balloon in a solvent to soften the balloon.

**6.** The method of claim **5**, wherein the solvent is acetone.

**7.** The method of claim **1**, wherein after crimping the stent to the second diameter, the balloon pressure is kept at the first pressure value for a period of time.

**8.** The method of claim **1**, wherein after crimping the stent to the third diameter, the balloon pressure is kept at the second pressure value for a period of time.

**9.** The method of claim **1**, further comprising releasing the pressure from the balloon after crimping the stent to the third diameter.

**10.** The method of claim **1**, wherein the stent comprises a network of interconnecting struts with gaps between adjacent struts, wherein after the crimping steps the balloon extends into the gaps to enhance stent retention.

**11.** The method of claim **1**, wherein the balloon is deflated for a period of time.

**12.** A method for crimping a stent onto a balloon, comprising:

sliding a stent at a first diameter over a balloon that is not inflated;

placing the stent and balloon that is not inflated in a stent crimper;

crimping the stent to a second diameter that is less than the first diameter while the balloon is not inflated;

inflating the balloon to a pressure value after crimping the stent to the second diameter;

crimping the stent to a third diameter that is less than the second diameter after inflating the balloon; and



7

controlling the pressure inside the balloon below the pressure value when the stent is being crimped onto the balloon.

13. The method of claim 12, further comprising reducing an inner diameter of the crimper to the outer diameter of the stent before inflating the balloon with the fluid. 5

14. The method of claim 12, wherein the step of controlling includes releasing the fluid inside the balloon when the pressure exceeds the pressure value so that the pressure inside the balloon does not exceed the pressure value. 10

15. The method of claim 14, wherein the step of releasing includes using a pressure release valve to control the fluid inside the balloon below the pressure value.

16. The method of claim 12, further comprising soaking the balloon in a solvent to soften the balloon. 15

17. The method of claim 16, wherein the solvent is acetone.

8

18. The method of claim 12, wherein after inflating the balloon and before crimping the stent to the third diameter, the balloon pressure is kept at the pressure value for a period of time.

19. The method of claim 12, wherein after crimping the stent to the third diameter, the balloon pressure is kept at the pressure value for a period of time.

20. The method of claim 12, further comprising releasing the pressure from the balloon after crimping the stent to the third diameter. 10

21. The method of claim 12, wherein the stent comprises a network of interconnecting struts with gaps between adjacent struts, wherein after the crimping steps the balloon extends into the gaps to enhance stent retention.

\* \* \* \* \*