

US007962212B2

(12) **United States Patent**  
**Signoff et al.**

(10) **Patent No.:** **US 7,962,212 B2**  
(45) **Date of Patent:** **Jun. 14, 2011**

(54) **MULTIPLE BATTERY CONFIGURATIONS IN AN IMPLANTABLE MEDICAL DEVICE**

(75) Inventors: **David M. Signoff**, San Clemente, CA (US); **Marcus F. Julian**, Dana Point, CA (US)

(73) Assignee: **Cameron Health, Inc.**, San Clemente, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 495 days.

(21) Appl. No.: **11/833,163**

(22) Filed: **Aug. 2, 2007**

(65) **Prior Publication Data**

US 2009/0036943 A1 Feb. 5, 2009

(51) **Int. Cl.**  
**A61N 1/08** (2006.01)

(52) **U.S. Cl.** ..... **607/34; 320/121**

(58) **Field of Classification Search** ..... **607/34, 607/5, 7; 320/121**  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,412,137 A	10/1983	Hansen et al.
5,369,351 A	11/1994	Adams
5,385,575 A	1/1995	Adams
5,439,482 A	8/1995	Adams et al.
5,749,904 A	5/1998	Gliner et al.
6,038,473 A	3/2000	Olson et al.

6,778,860 B2	8/2004	Ostroff et al.
6,954,669 B1	10/2005	Fishler et al.
2003/0088277 A1	5/2003	Ostroff
2004/0193227 A1	9/2004	Schmidt
2005/0021094 A1	1/2005	Ostroff et al.
2006/0111752 A1*	5/2006	Greatbatch et al. .... 607/34

**FOREIGN PATENT DOCUMENTS**

WO	2006 058028 A2	6/2006
WO	2006 061725 A2	6/2006

**OTHER PUBLICATIONS**

Buchmann, Isidor, "Serial and parallel battery configurations", BatteryUniversity.com.\*  
Office Action; dated Sep. 10, 2007; U.S. Appl. No. 10/913,037 (US 2005-0021094 A1—Ostroff, et al).  
International Search Report and Written Opinion for PCT/US2008/071976; issued Dec. 5, 2008.

\* cited by examiner

*Primary Examiner* — Mark W Bockelman


*Assistant Examiner* — Erica Lee



(74) *Attorney, Agent, or Firm* — Pramudji Law Group PLLC; Ari Pramudji; Mark Schroeder

(57) **ABSTRACT**

Implantable medical device power circuits are disclosed. Multiple batteries may be provided, along with a number of switches, enabling a plurality of battery and power circuit configurations to be defined. Configurations of the power circuit may be changed in response to changes in battery status as the batteries are used and/or near end-of-life. Configurations of the power circuit may also be performed in response to changes in device operation. Methods associated with operating such circuits and implantable medical devices are also disclosed.

**13 Claims, 13 Drawing Sheets**

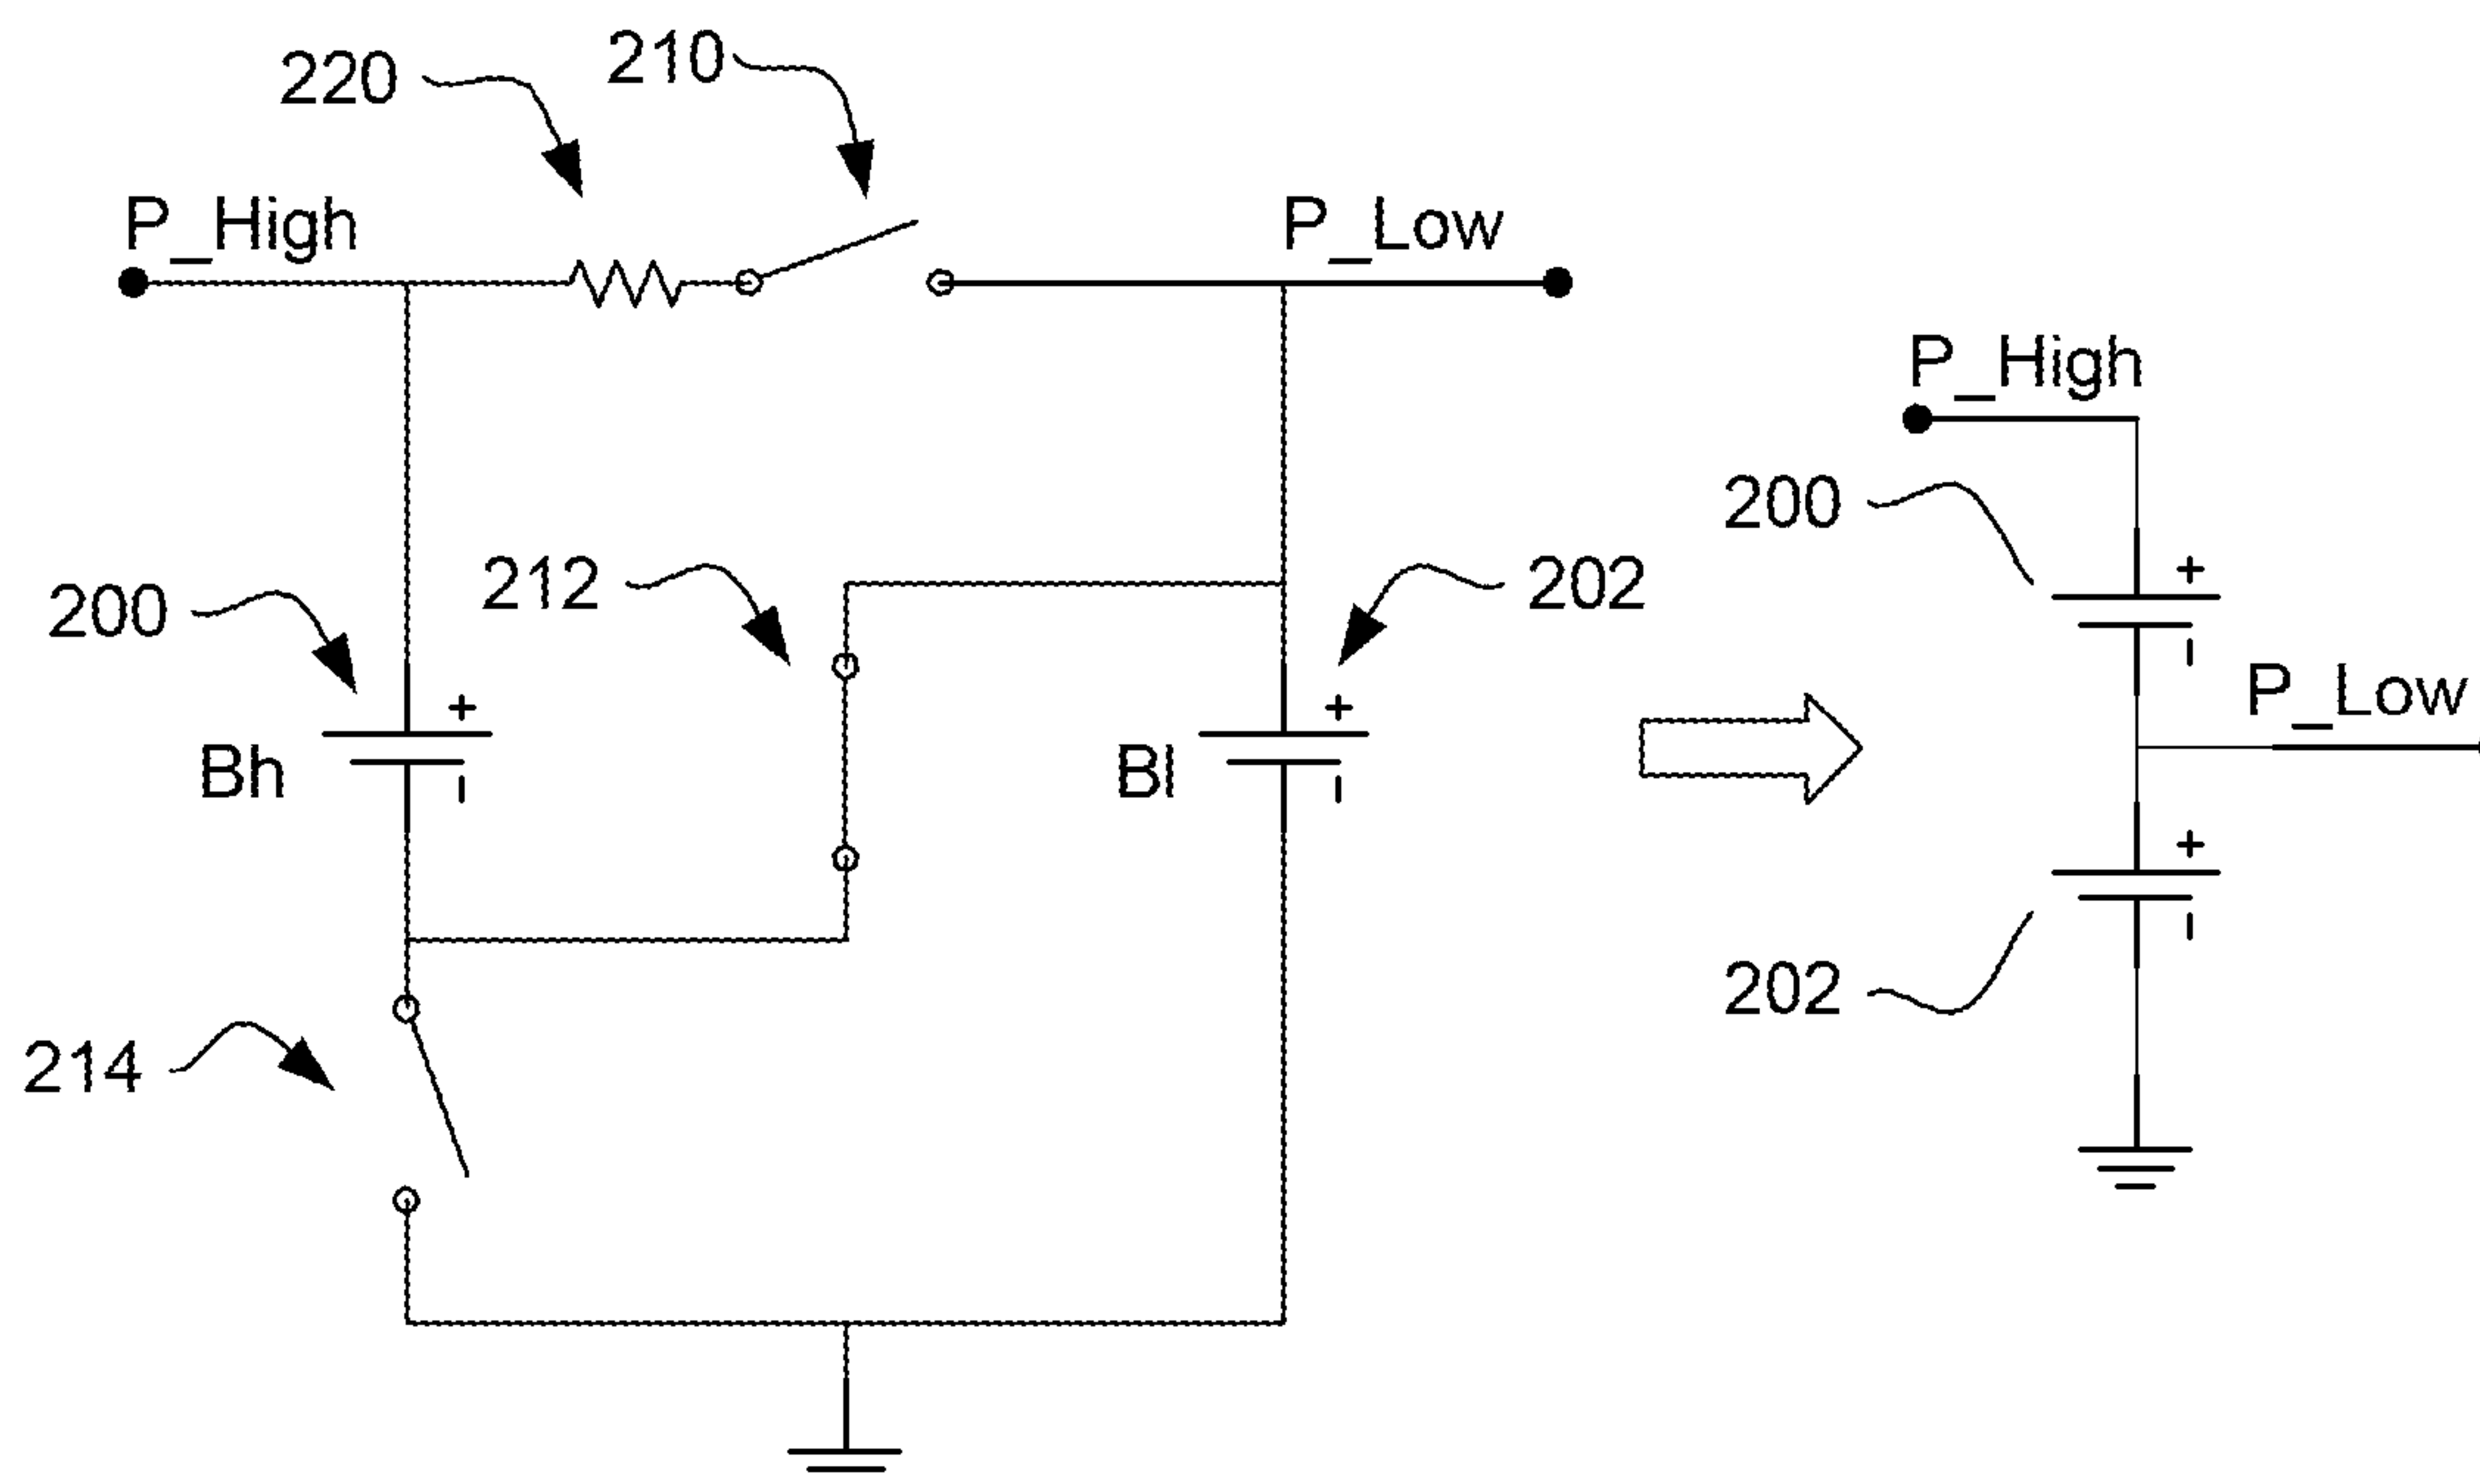

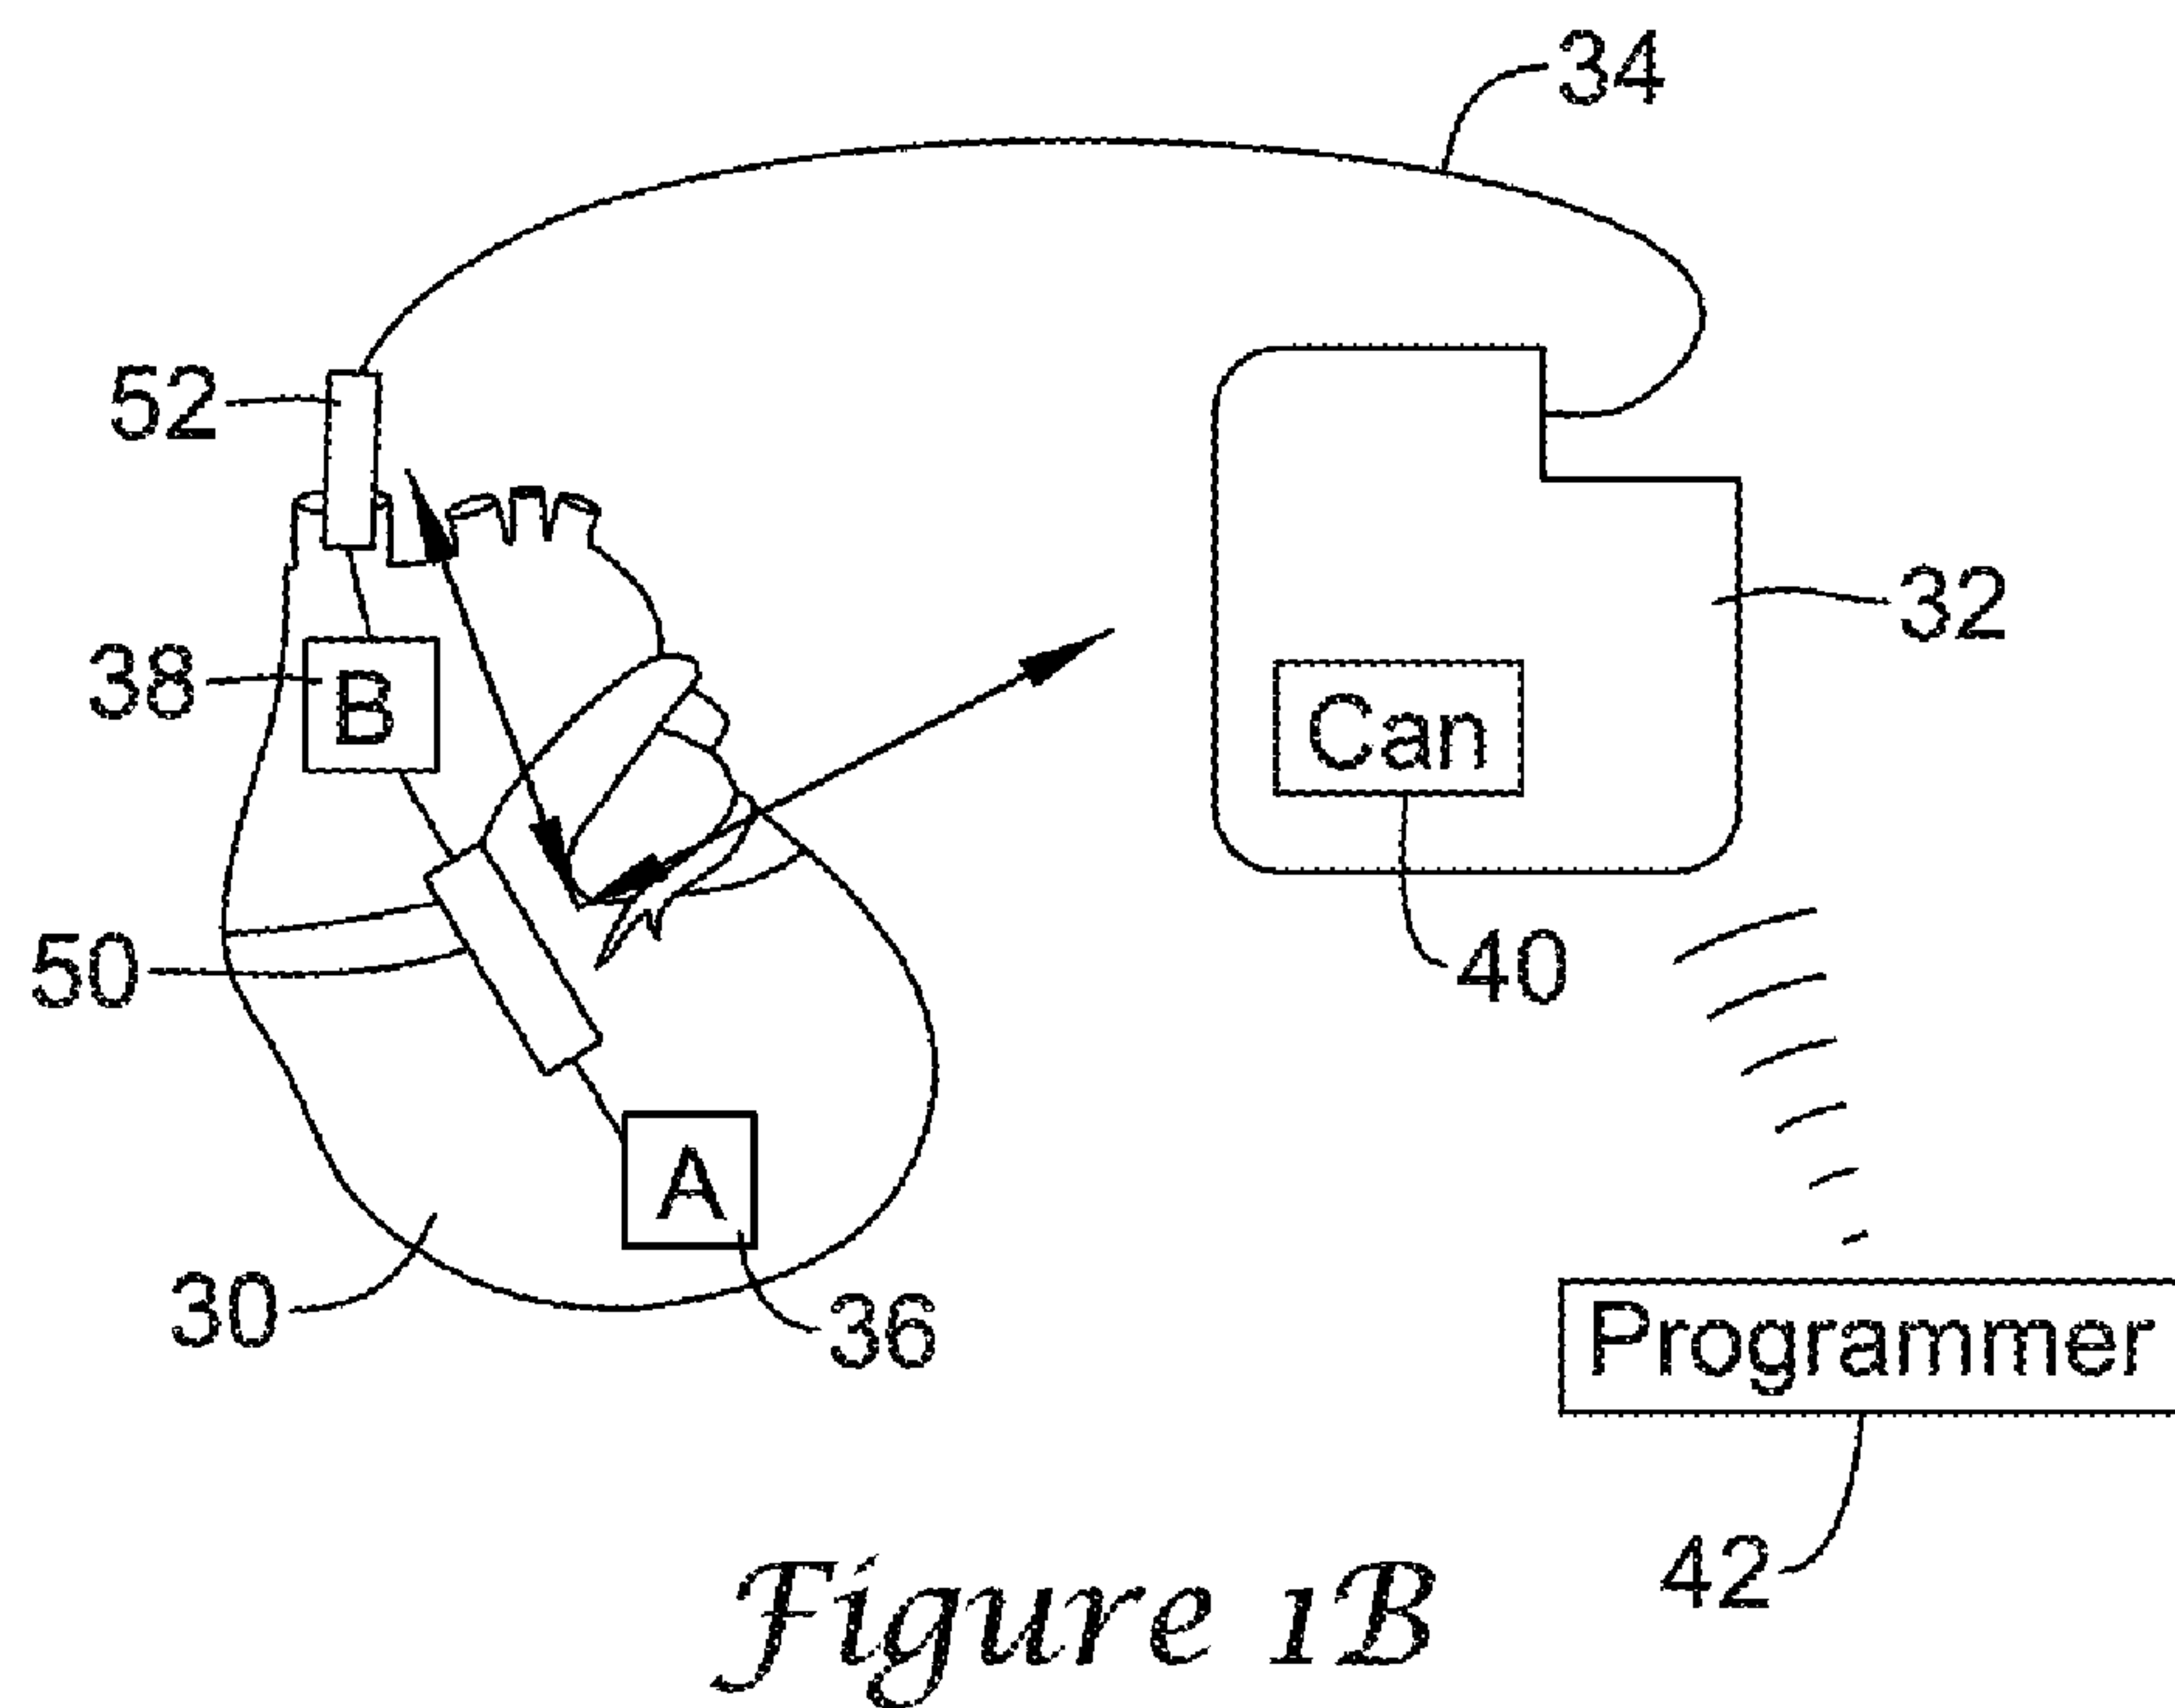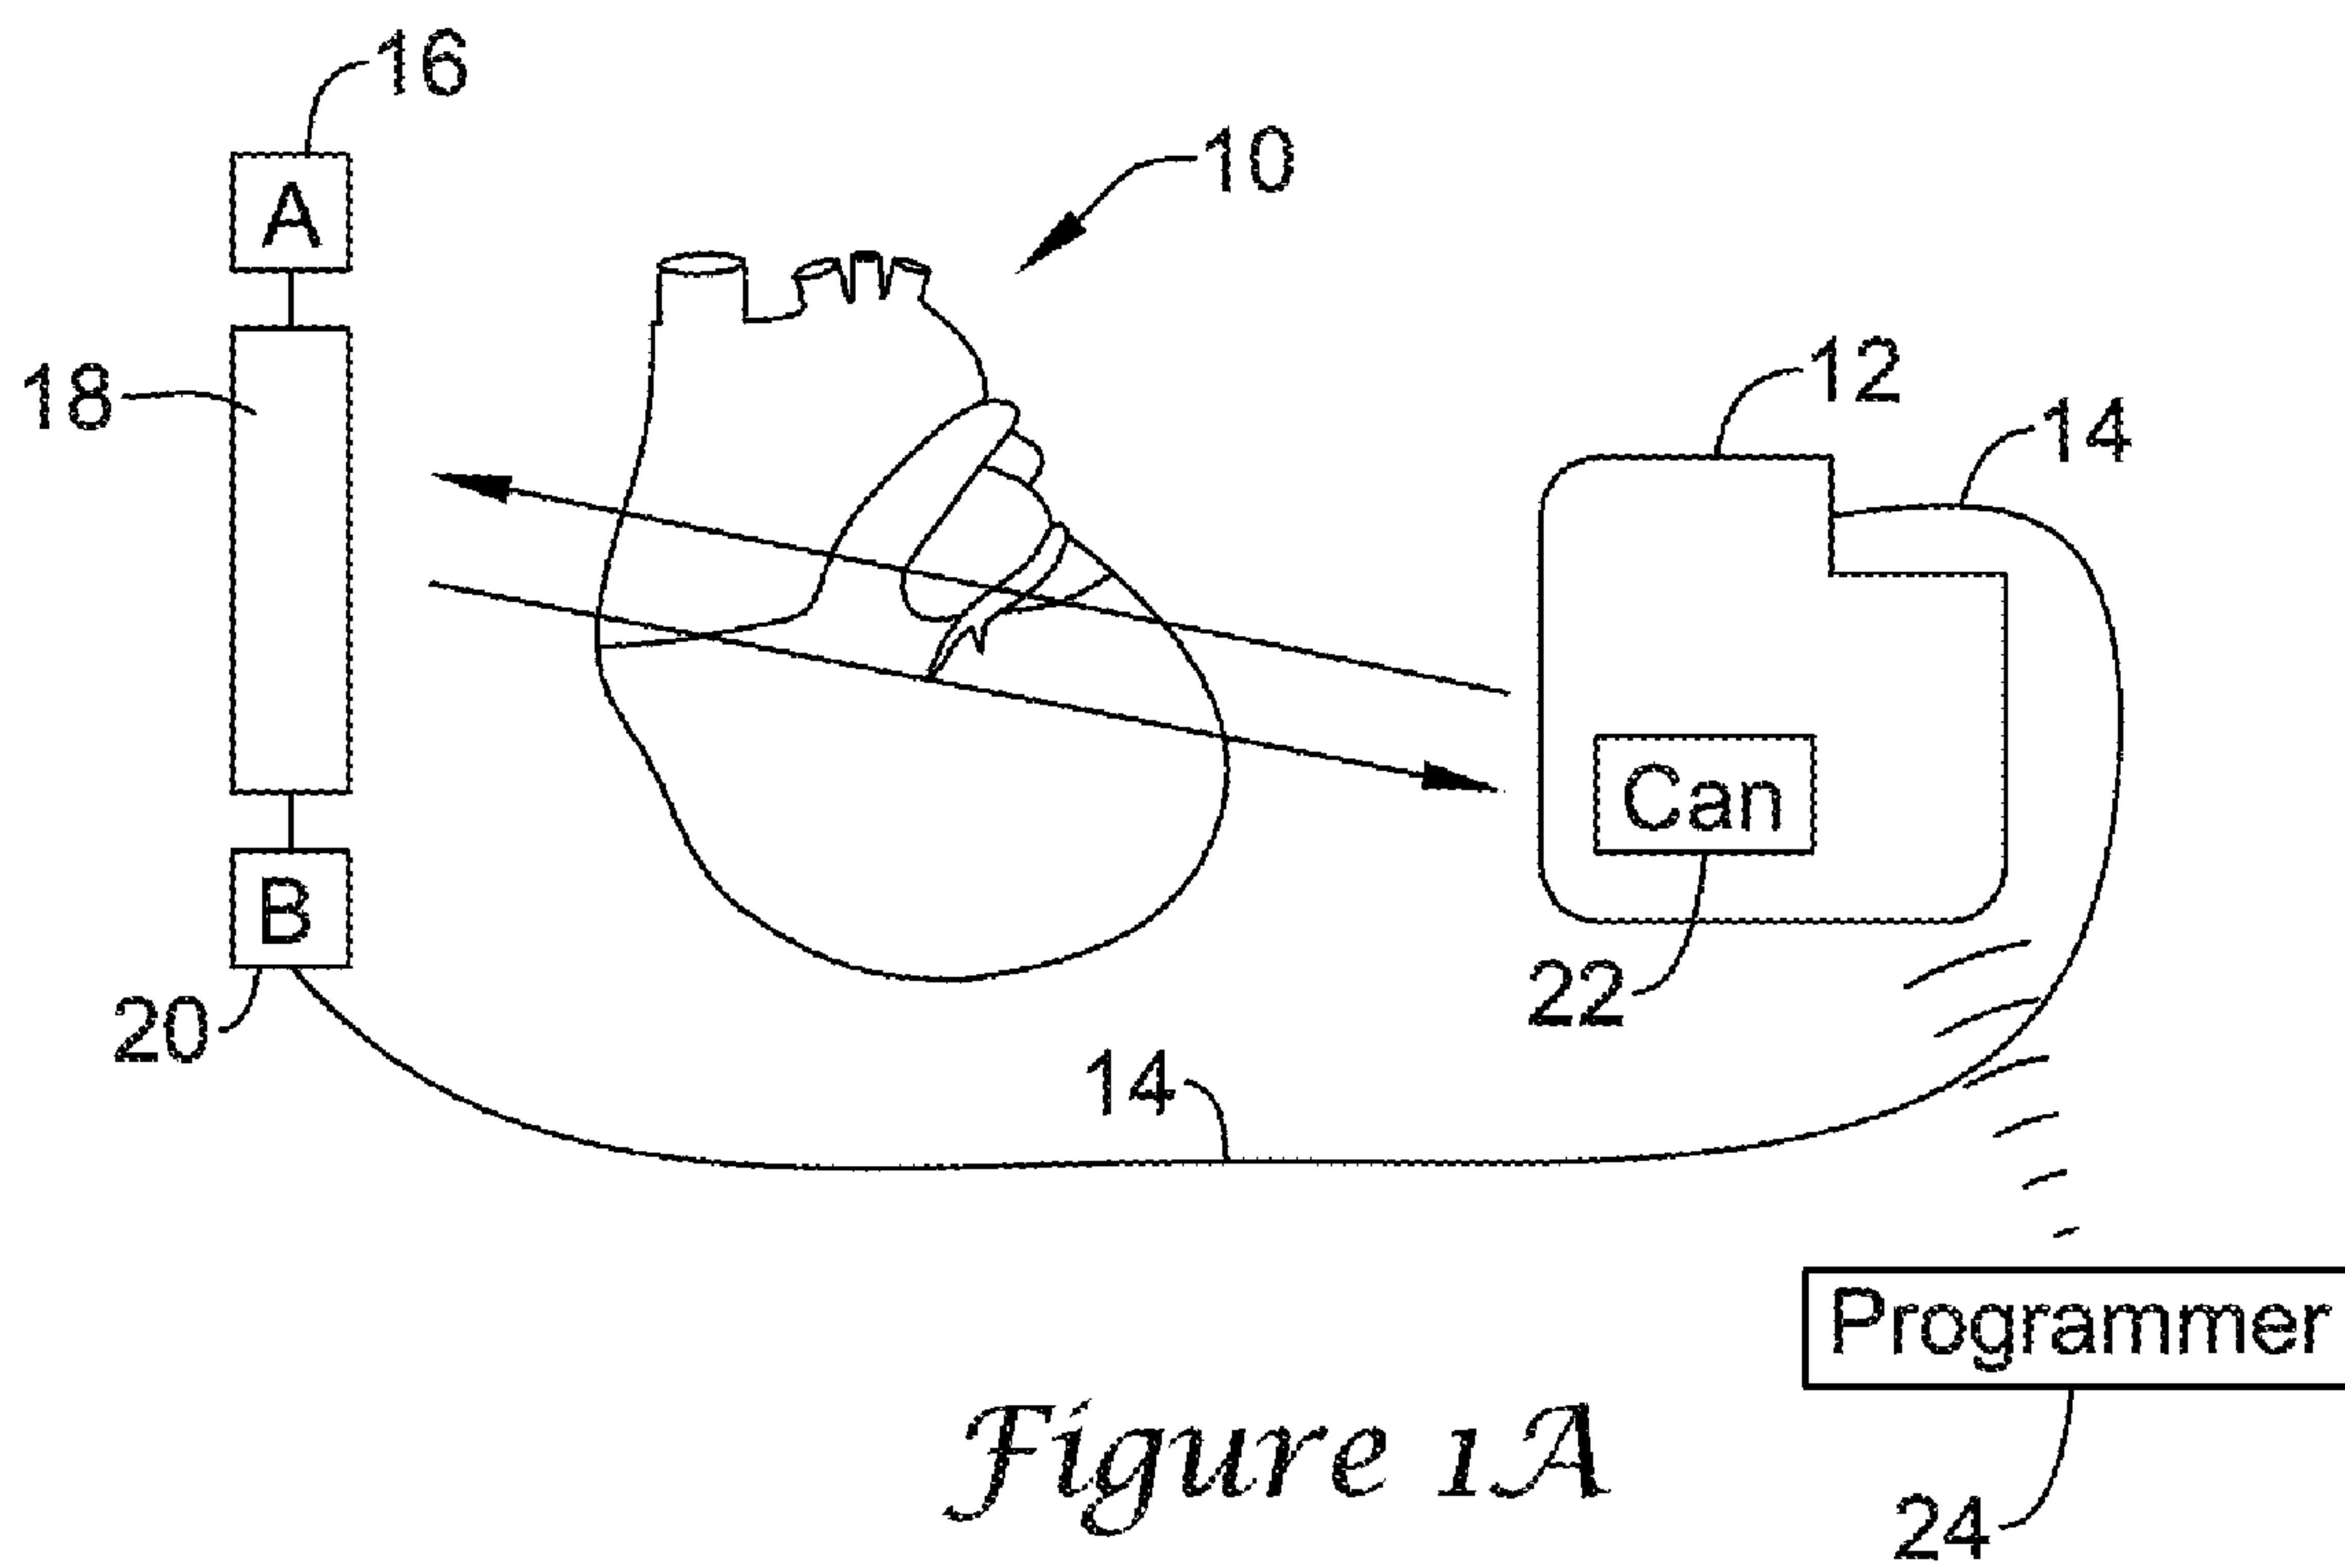

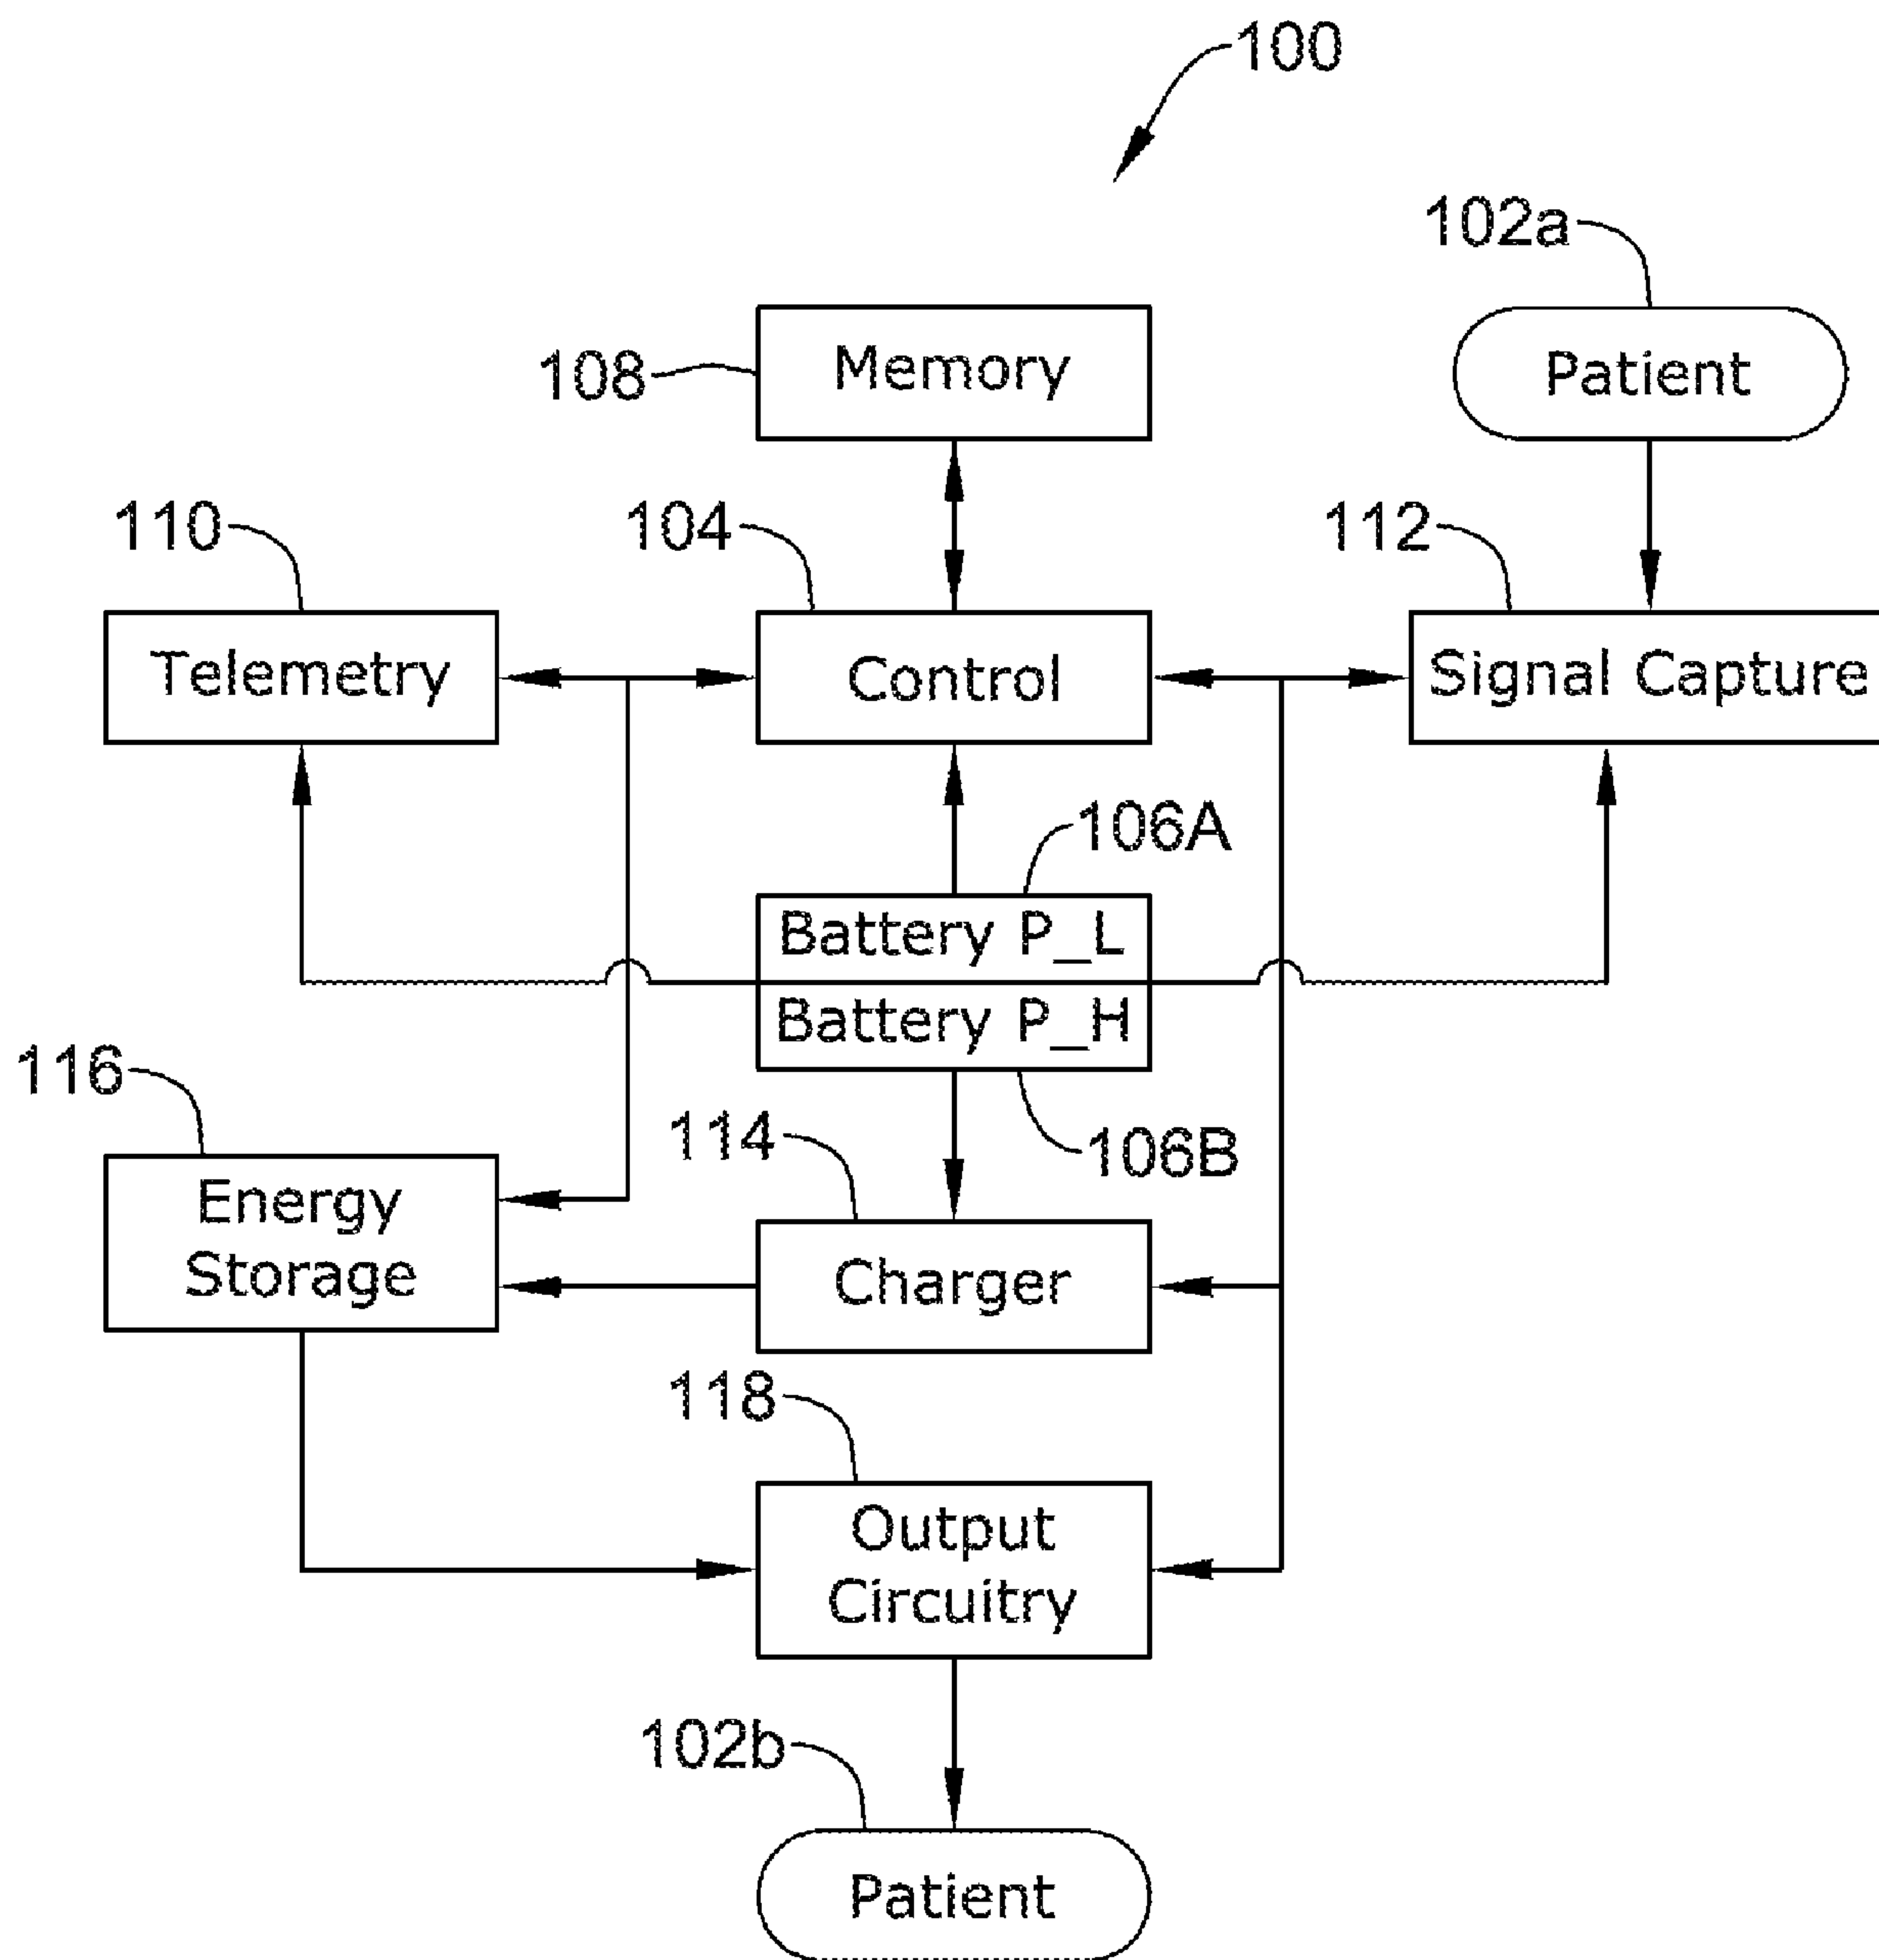


Figure 2

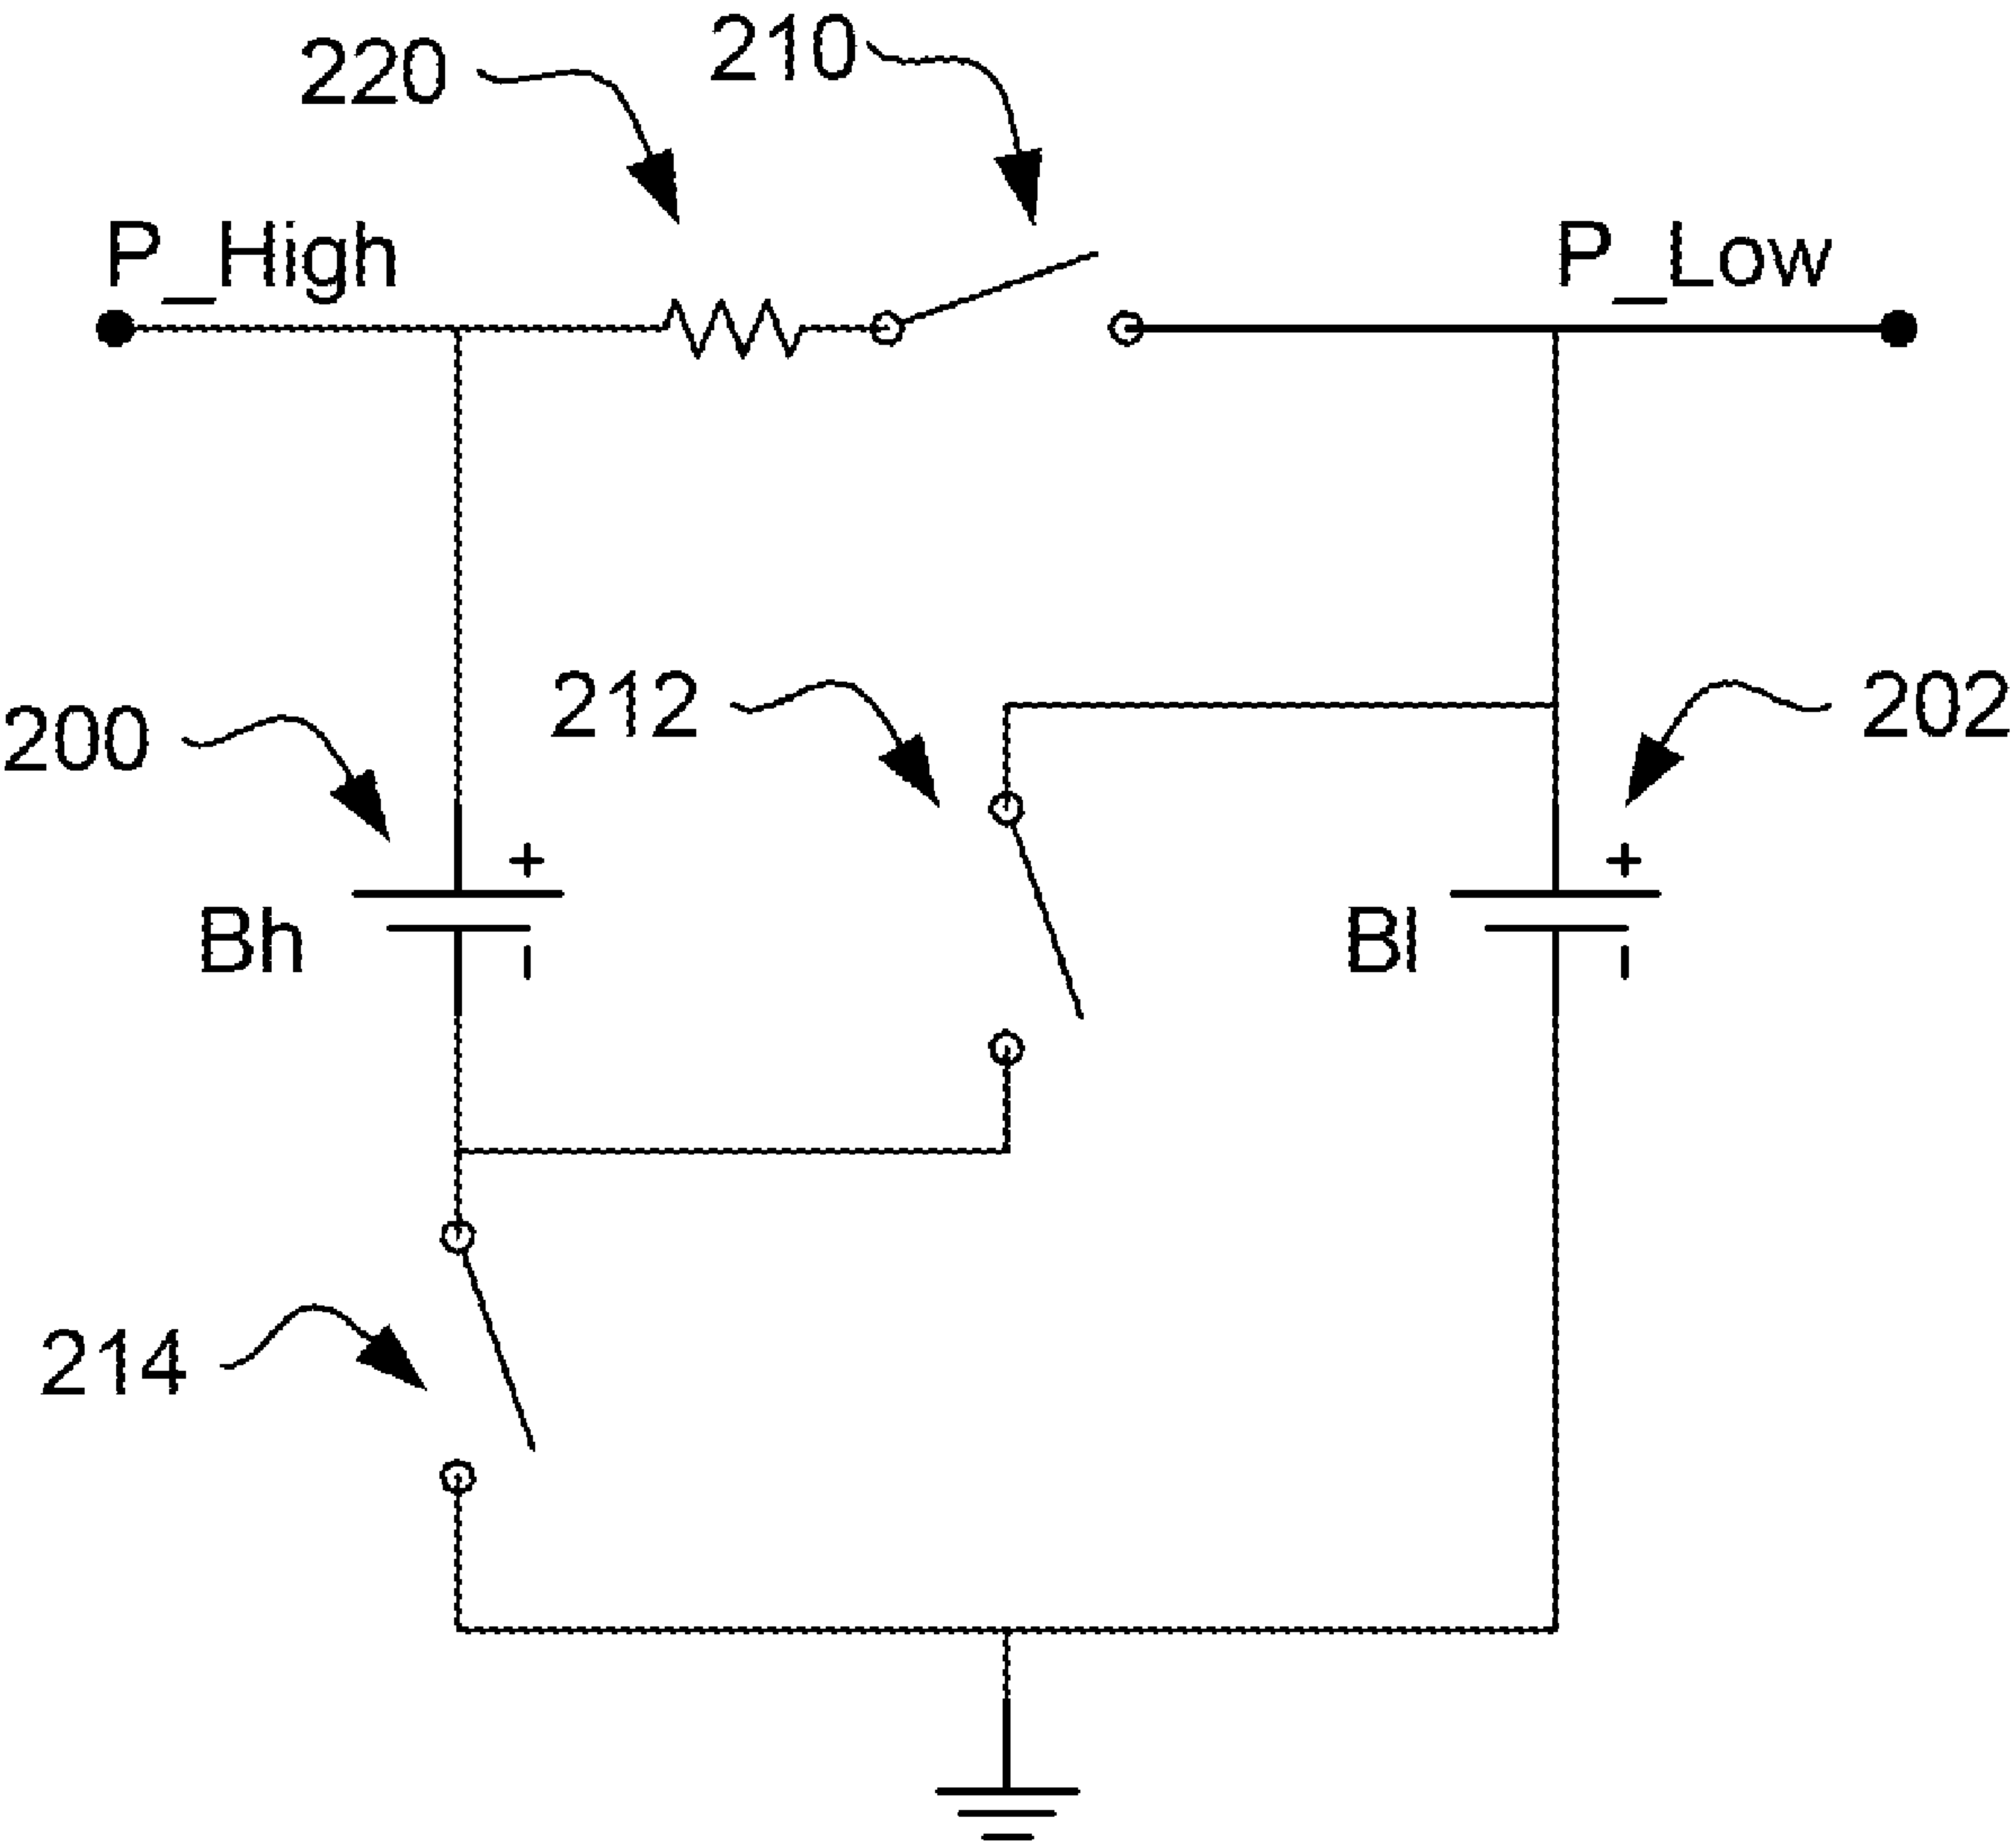


Figure 3


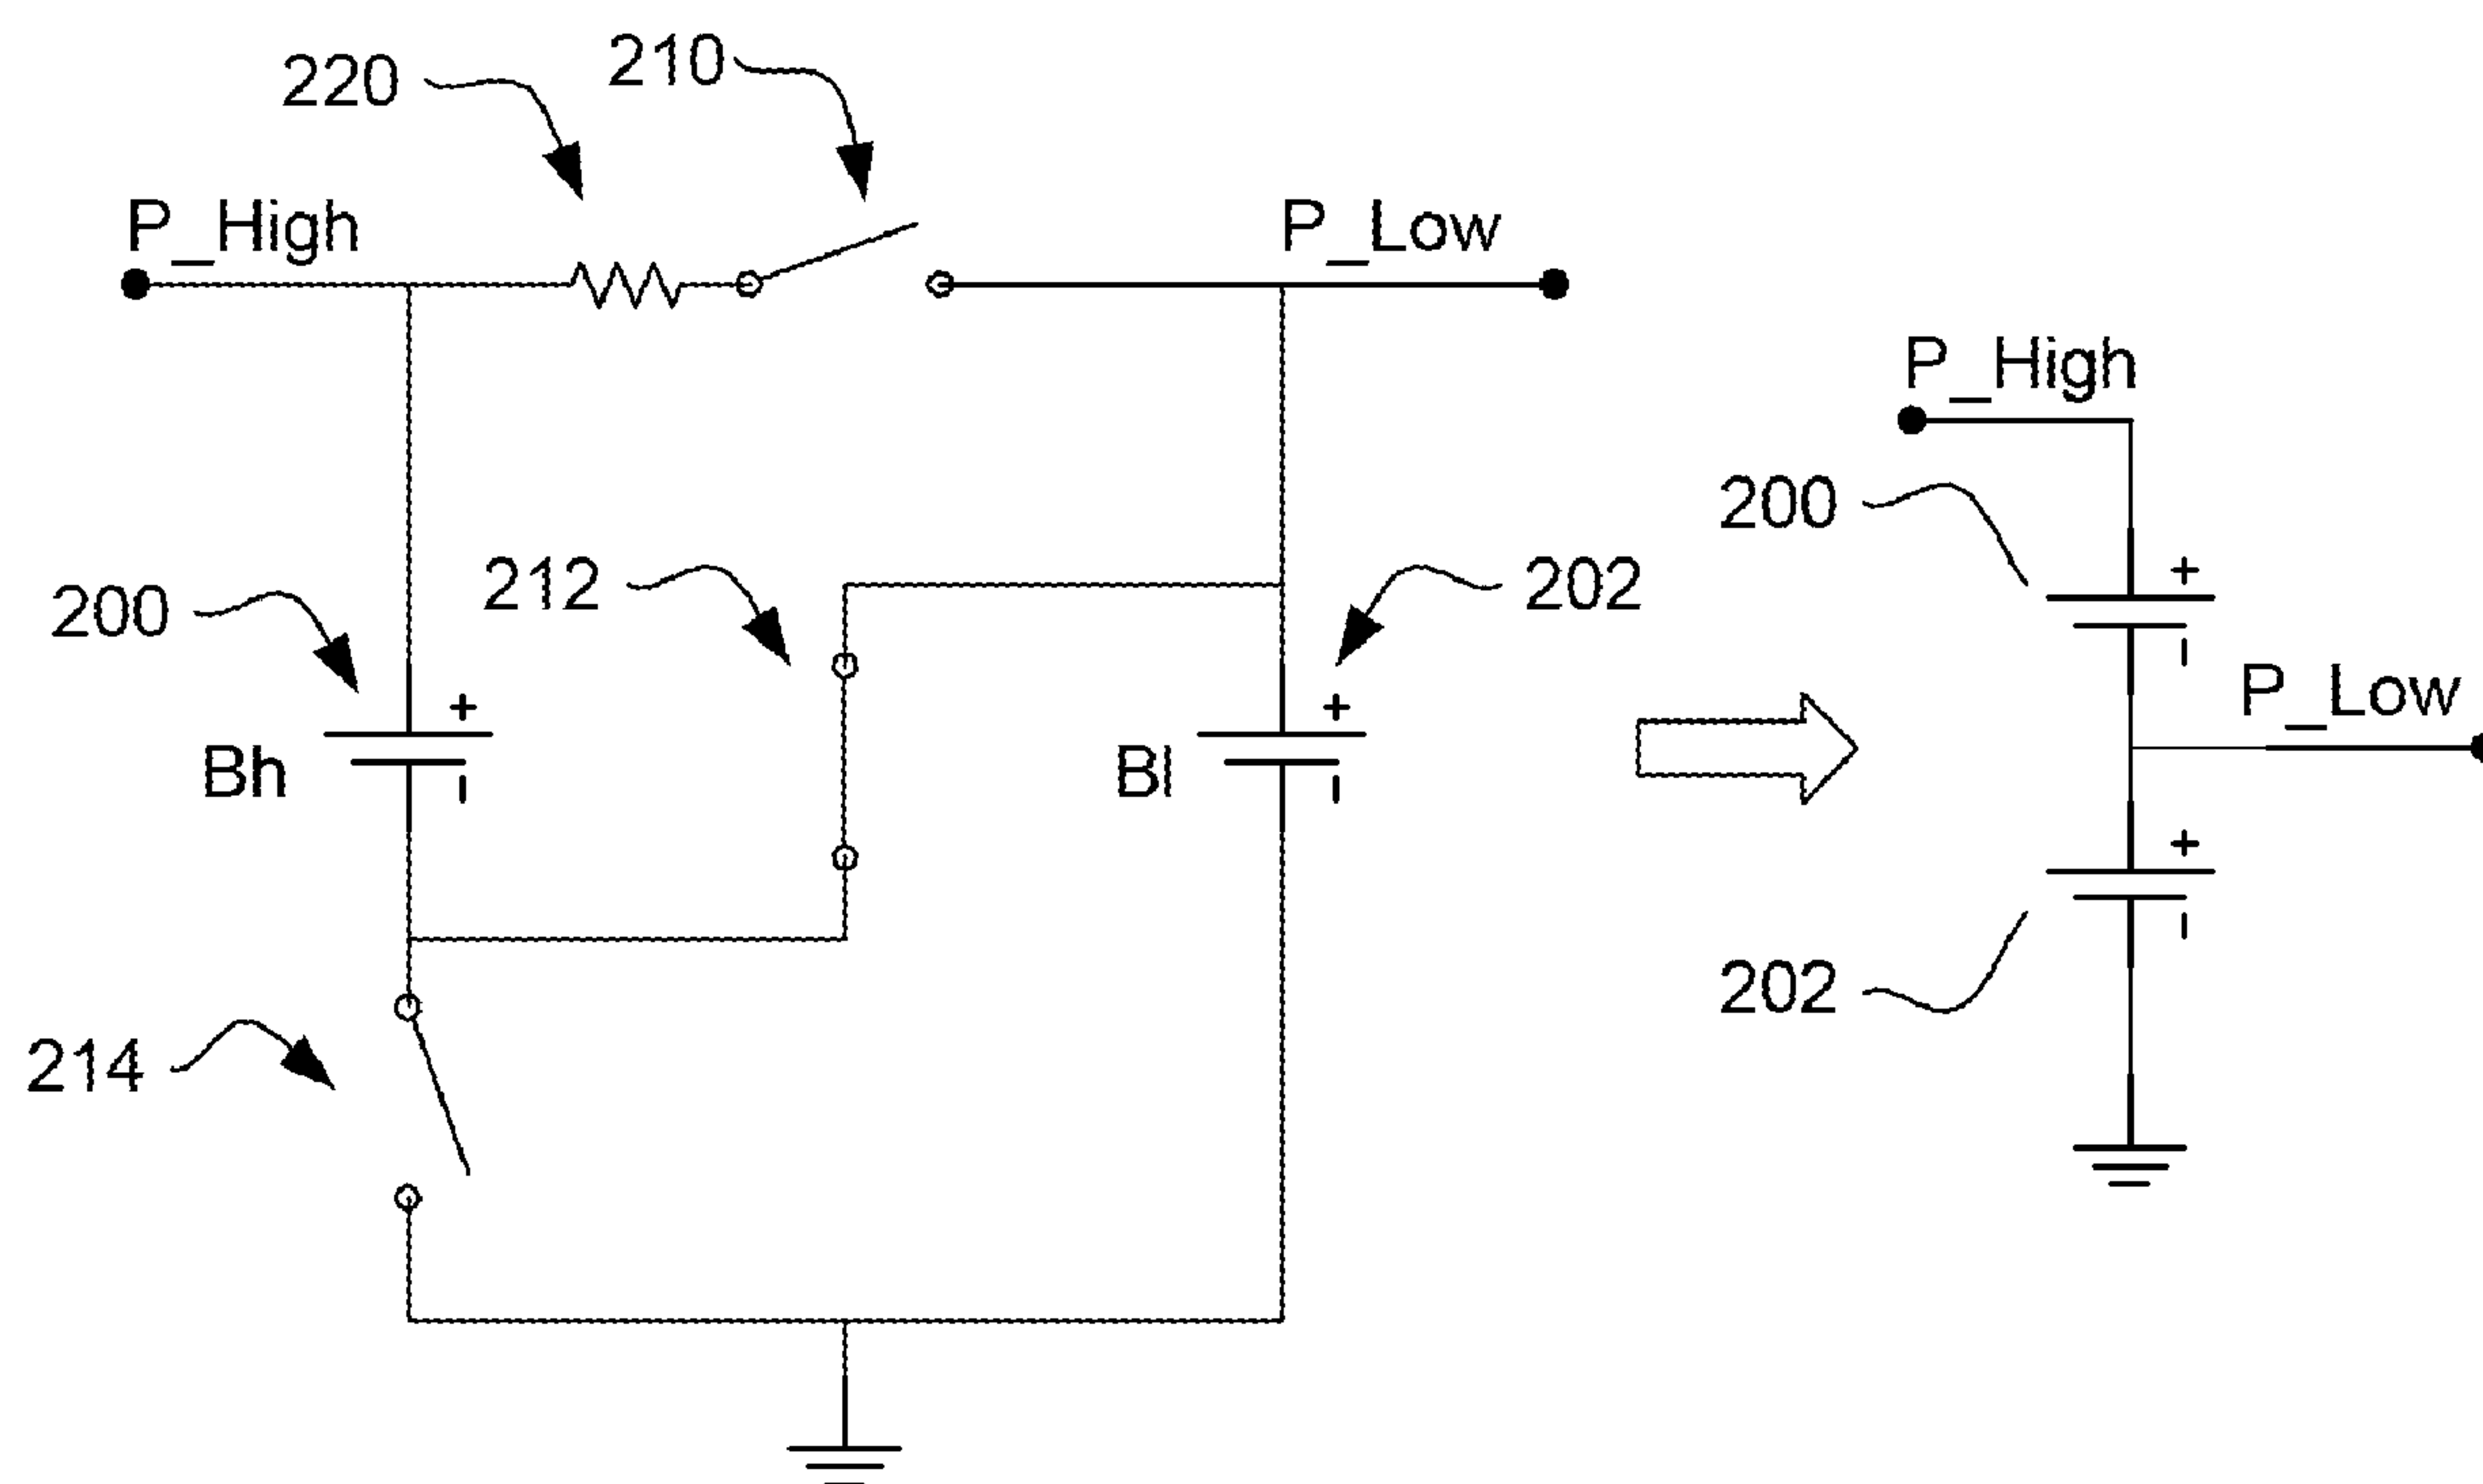


Figure 4A

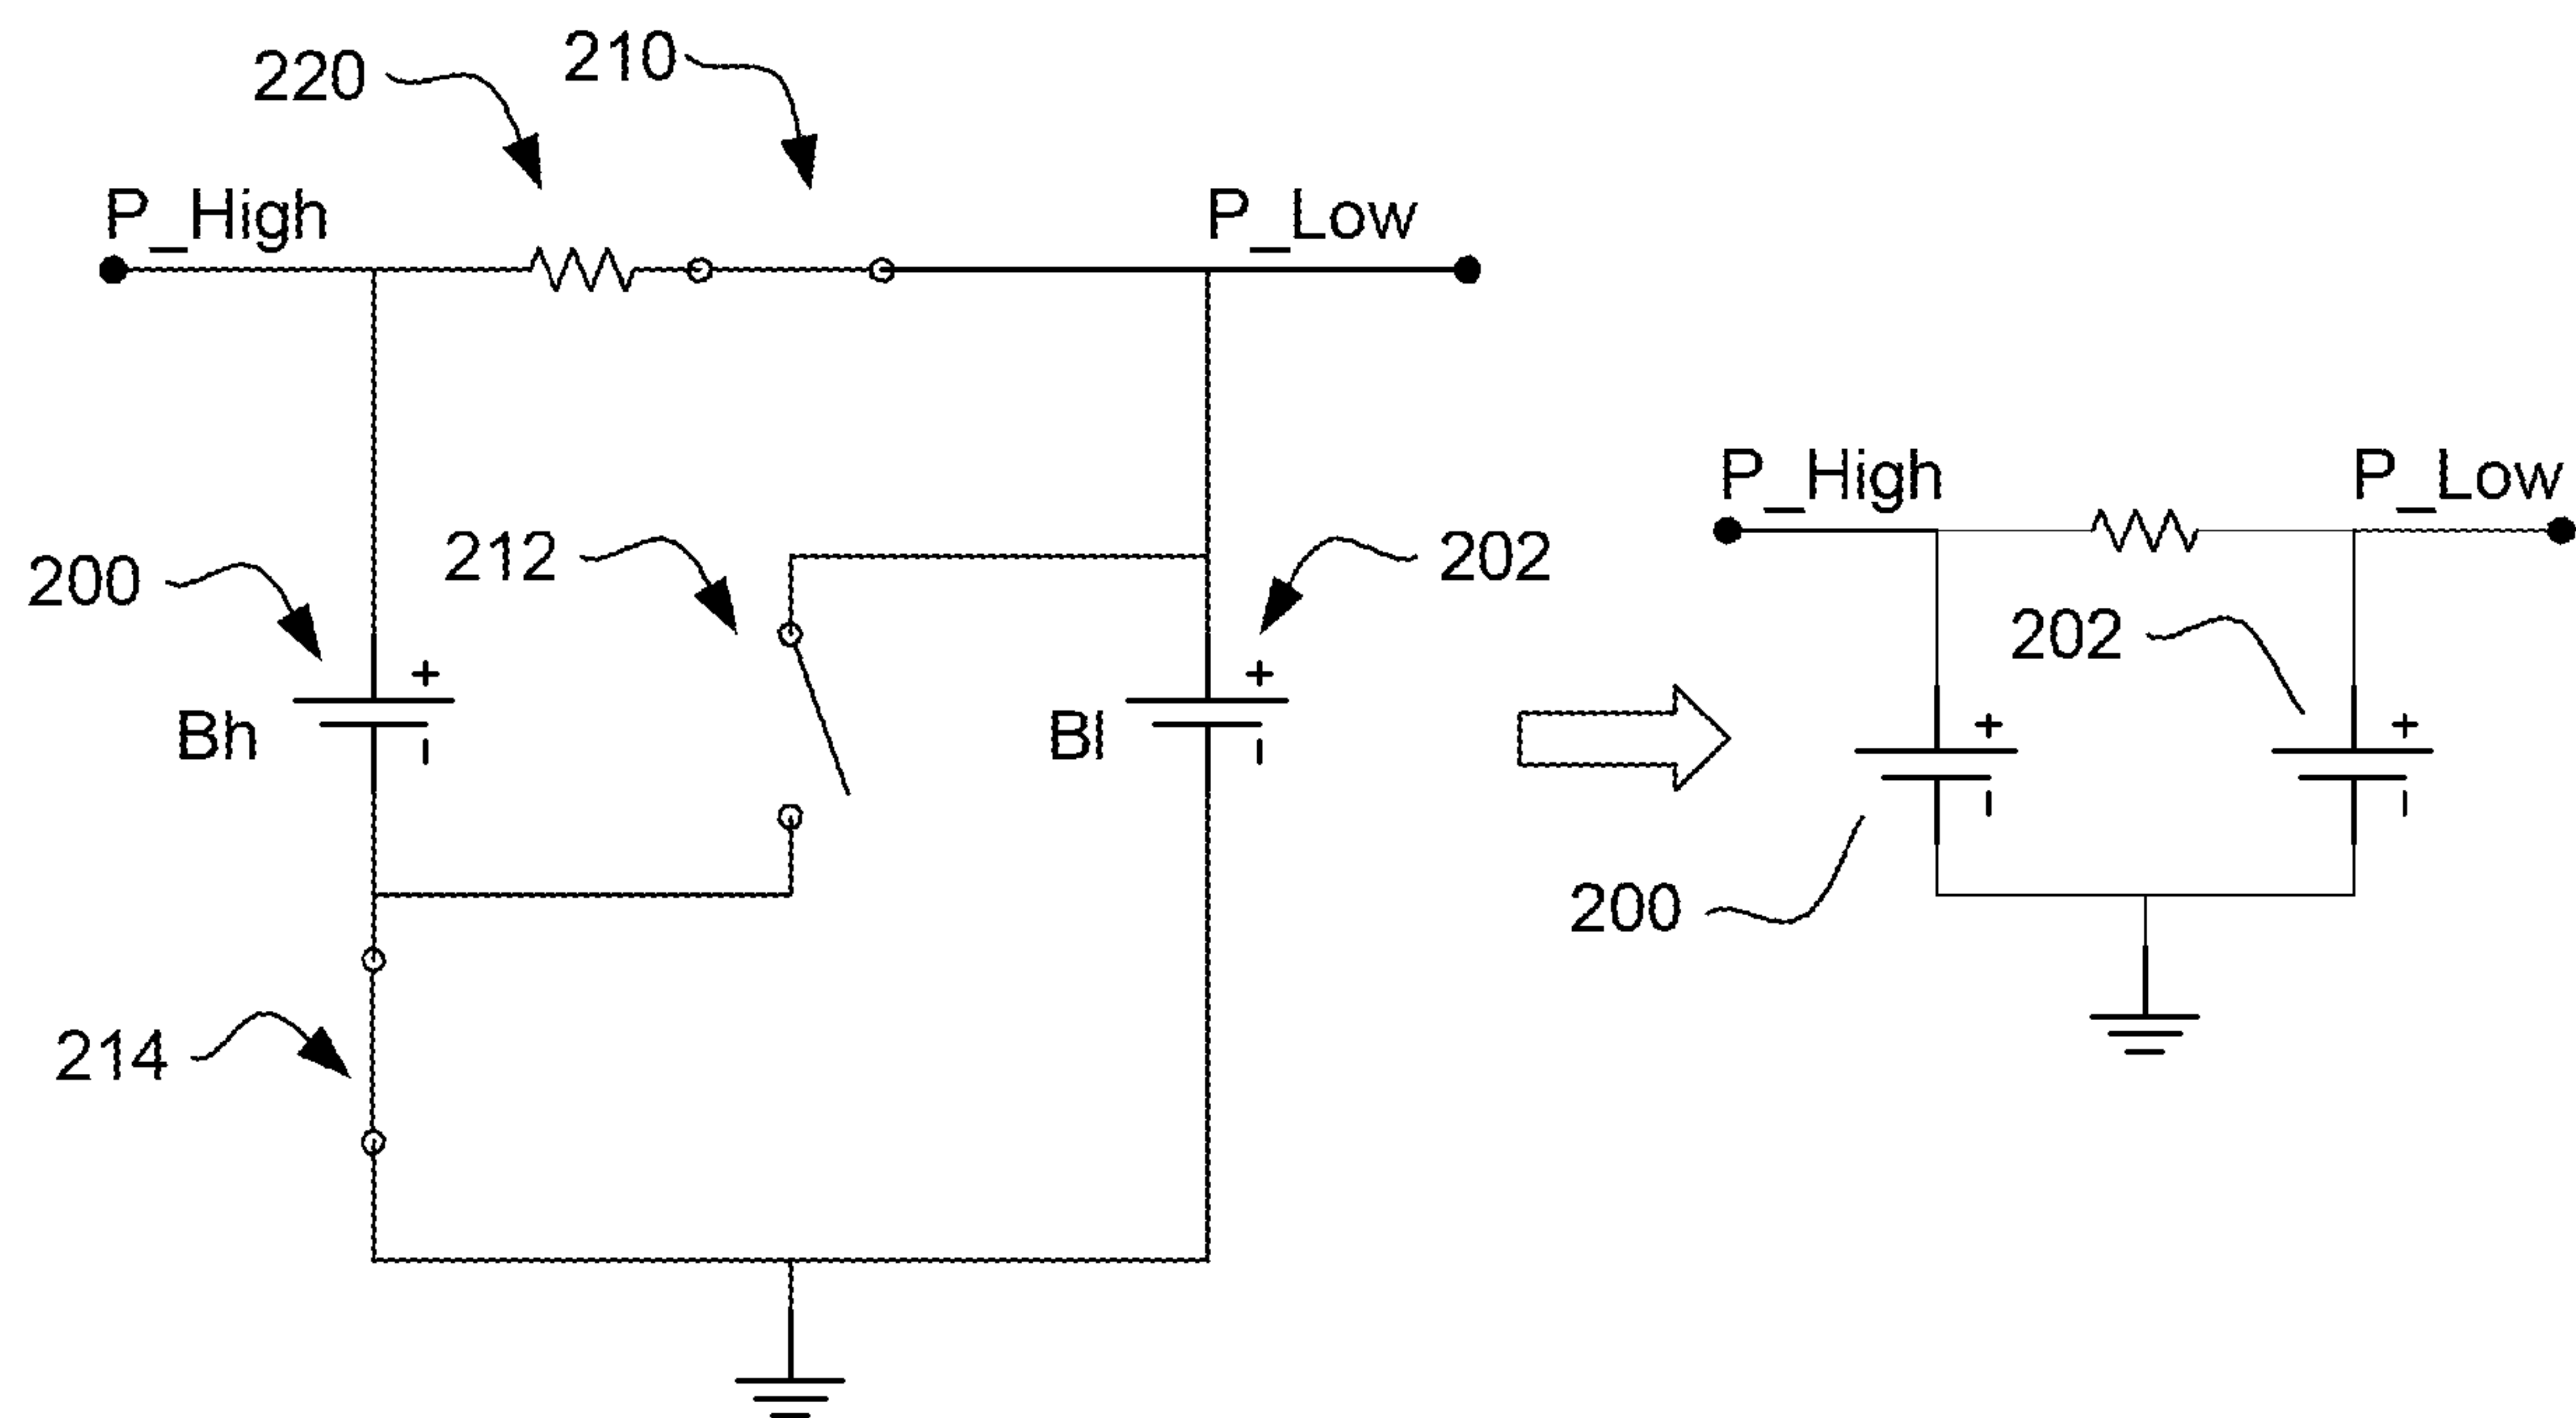

*Figure 4B*

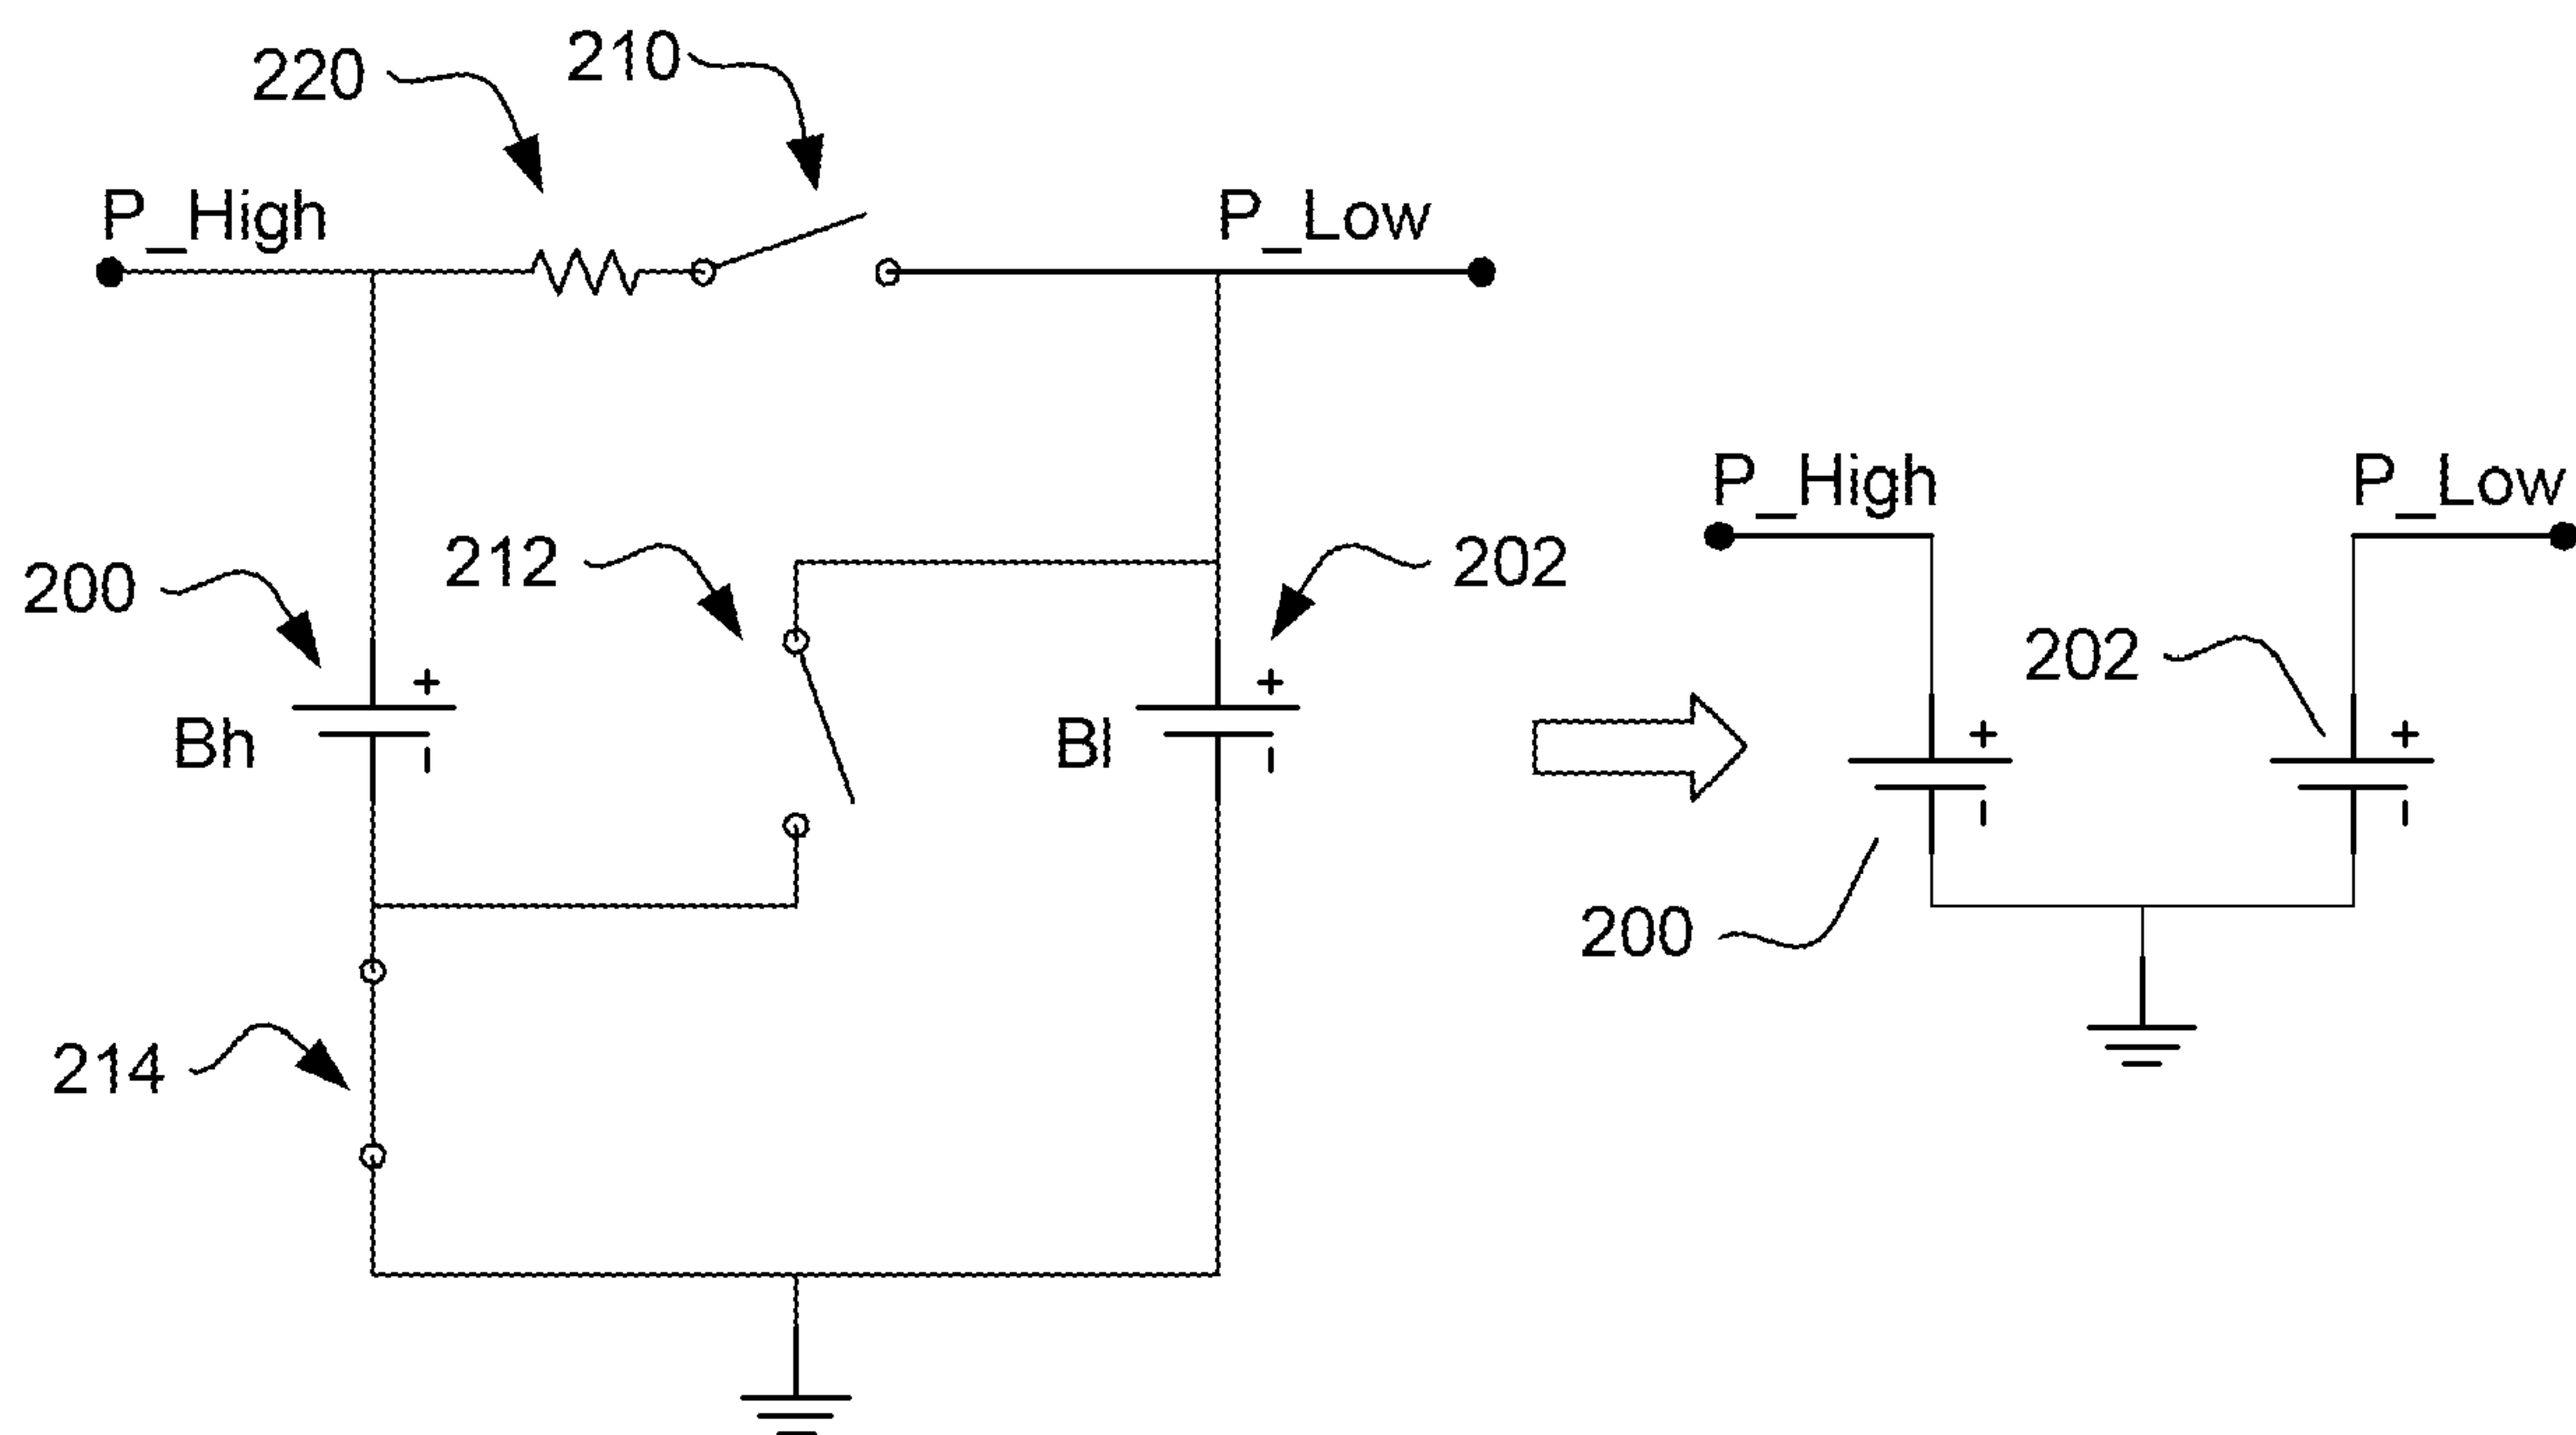


Figure 4C



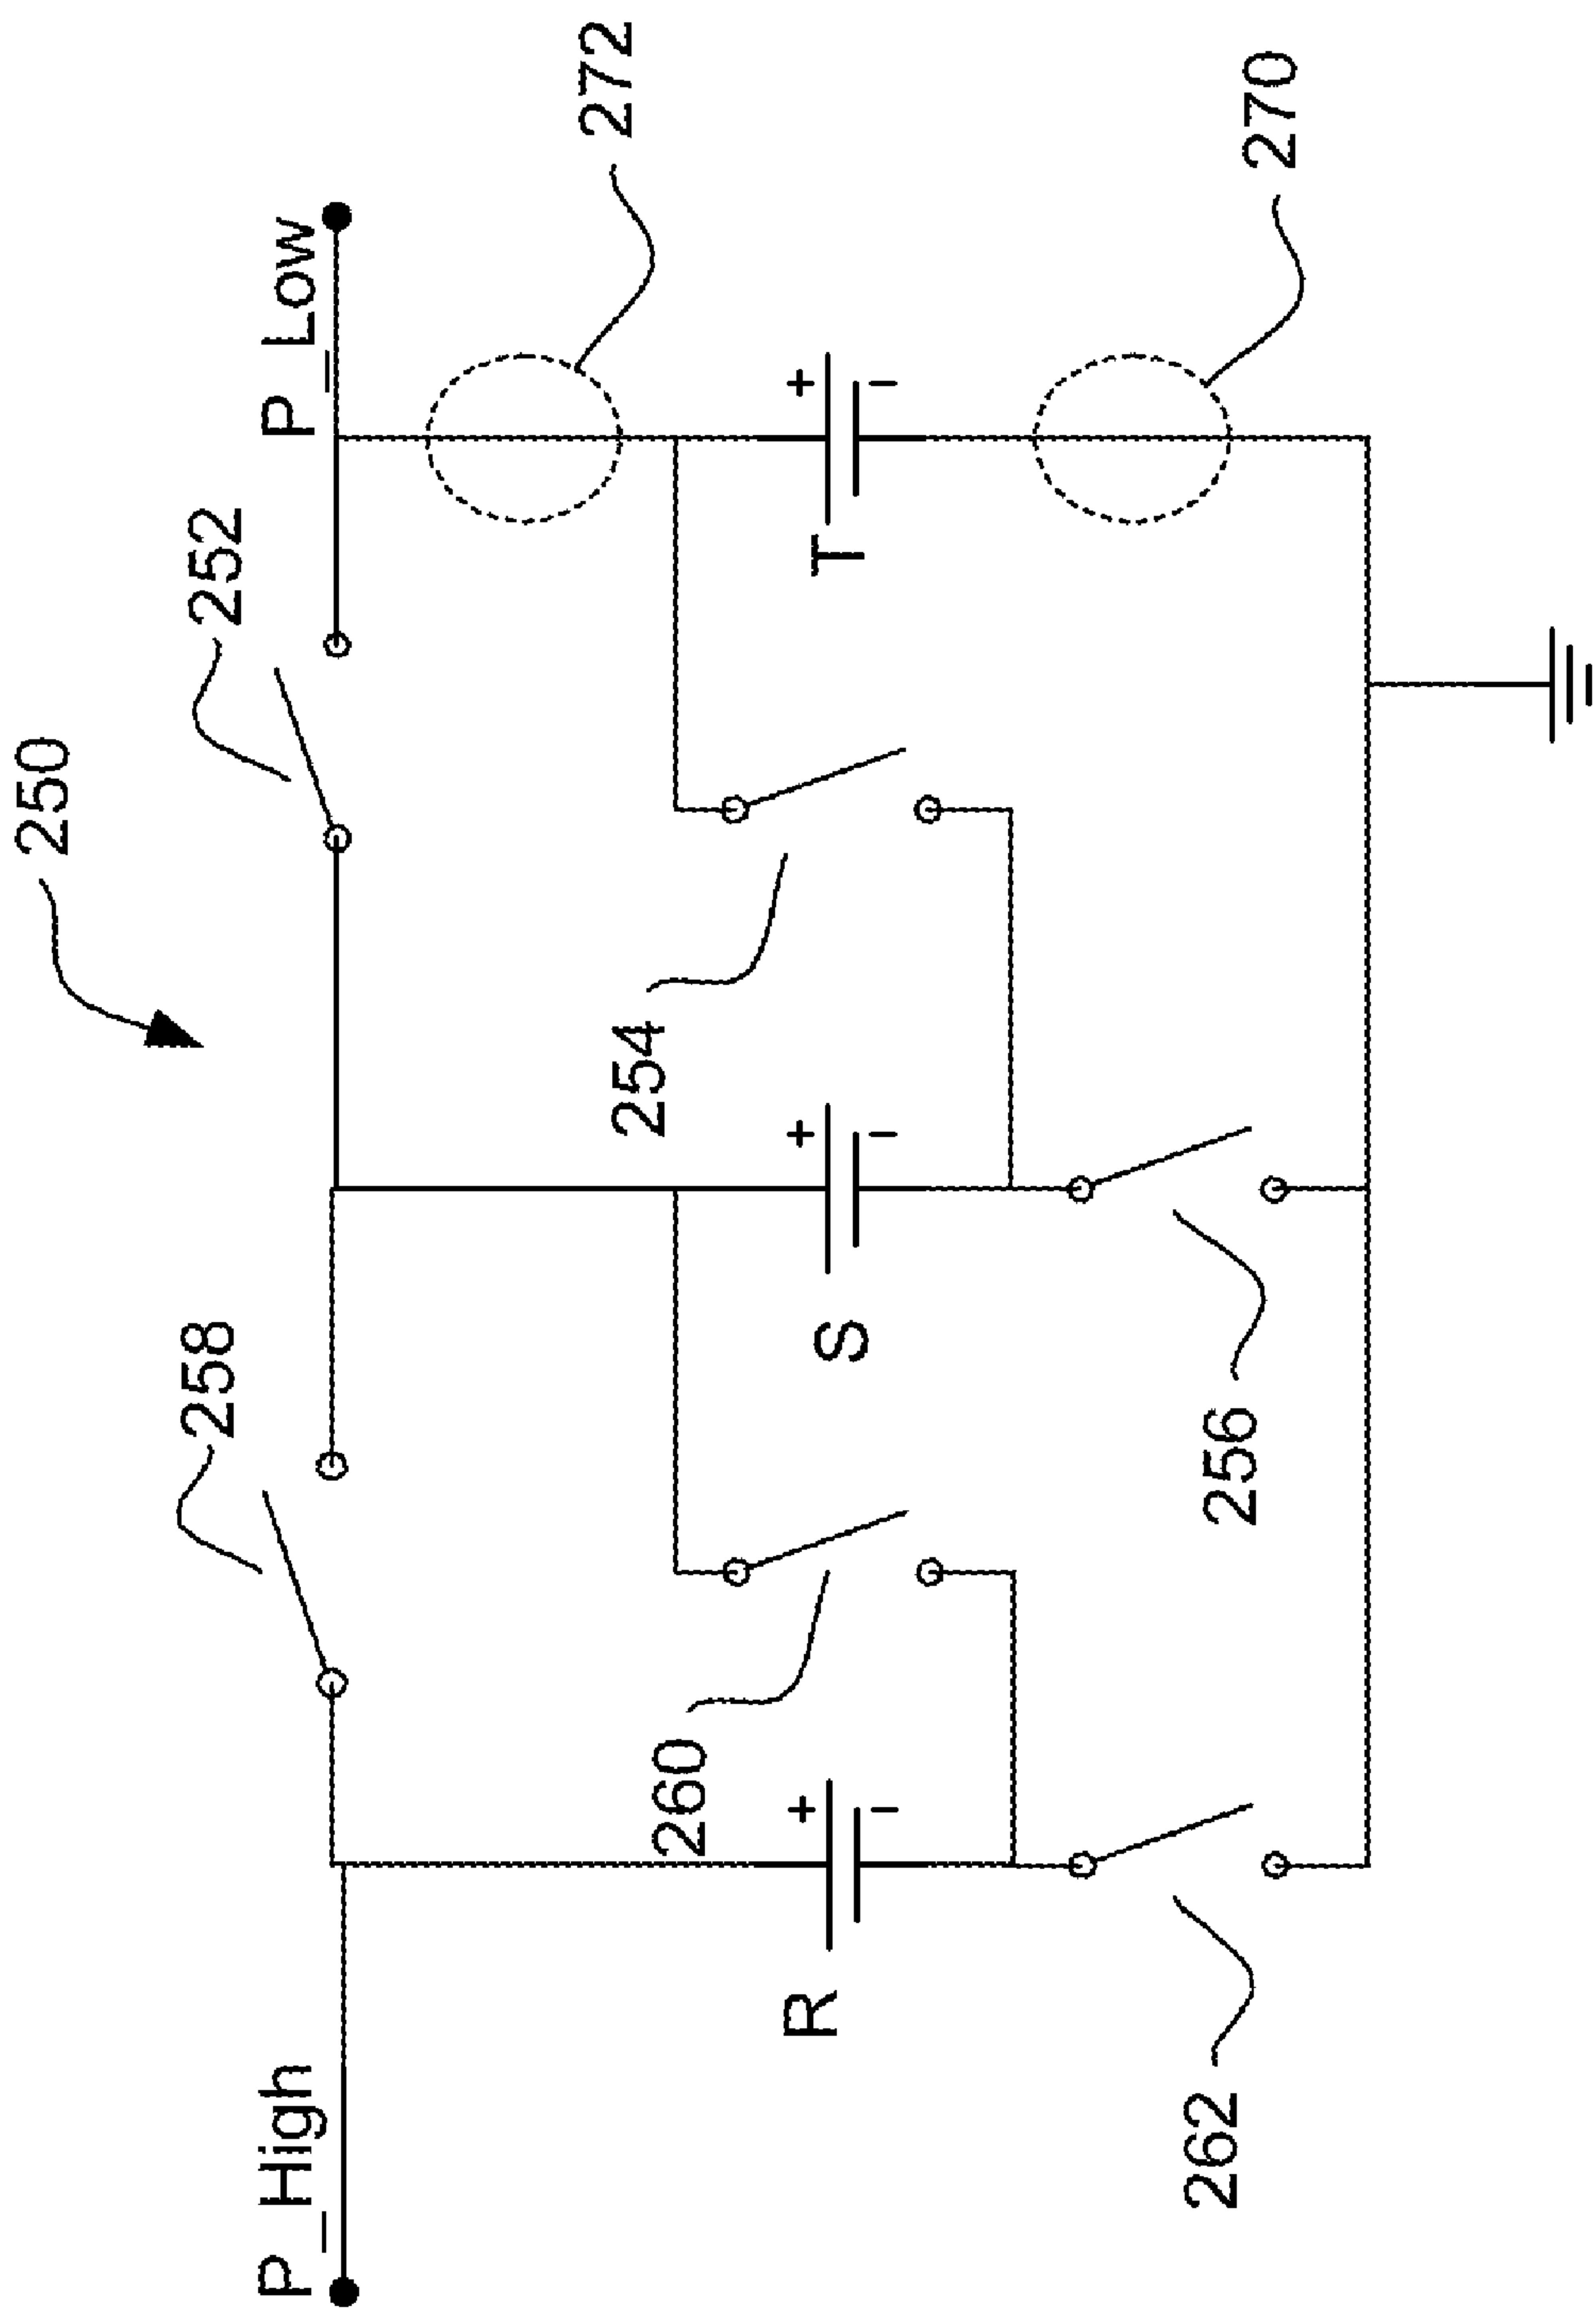



Figure 5

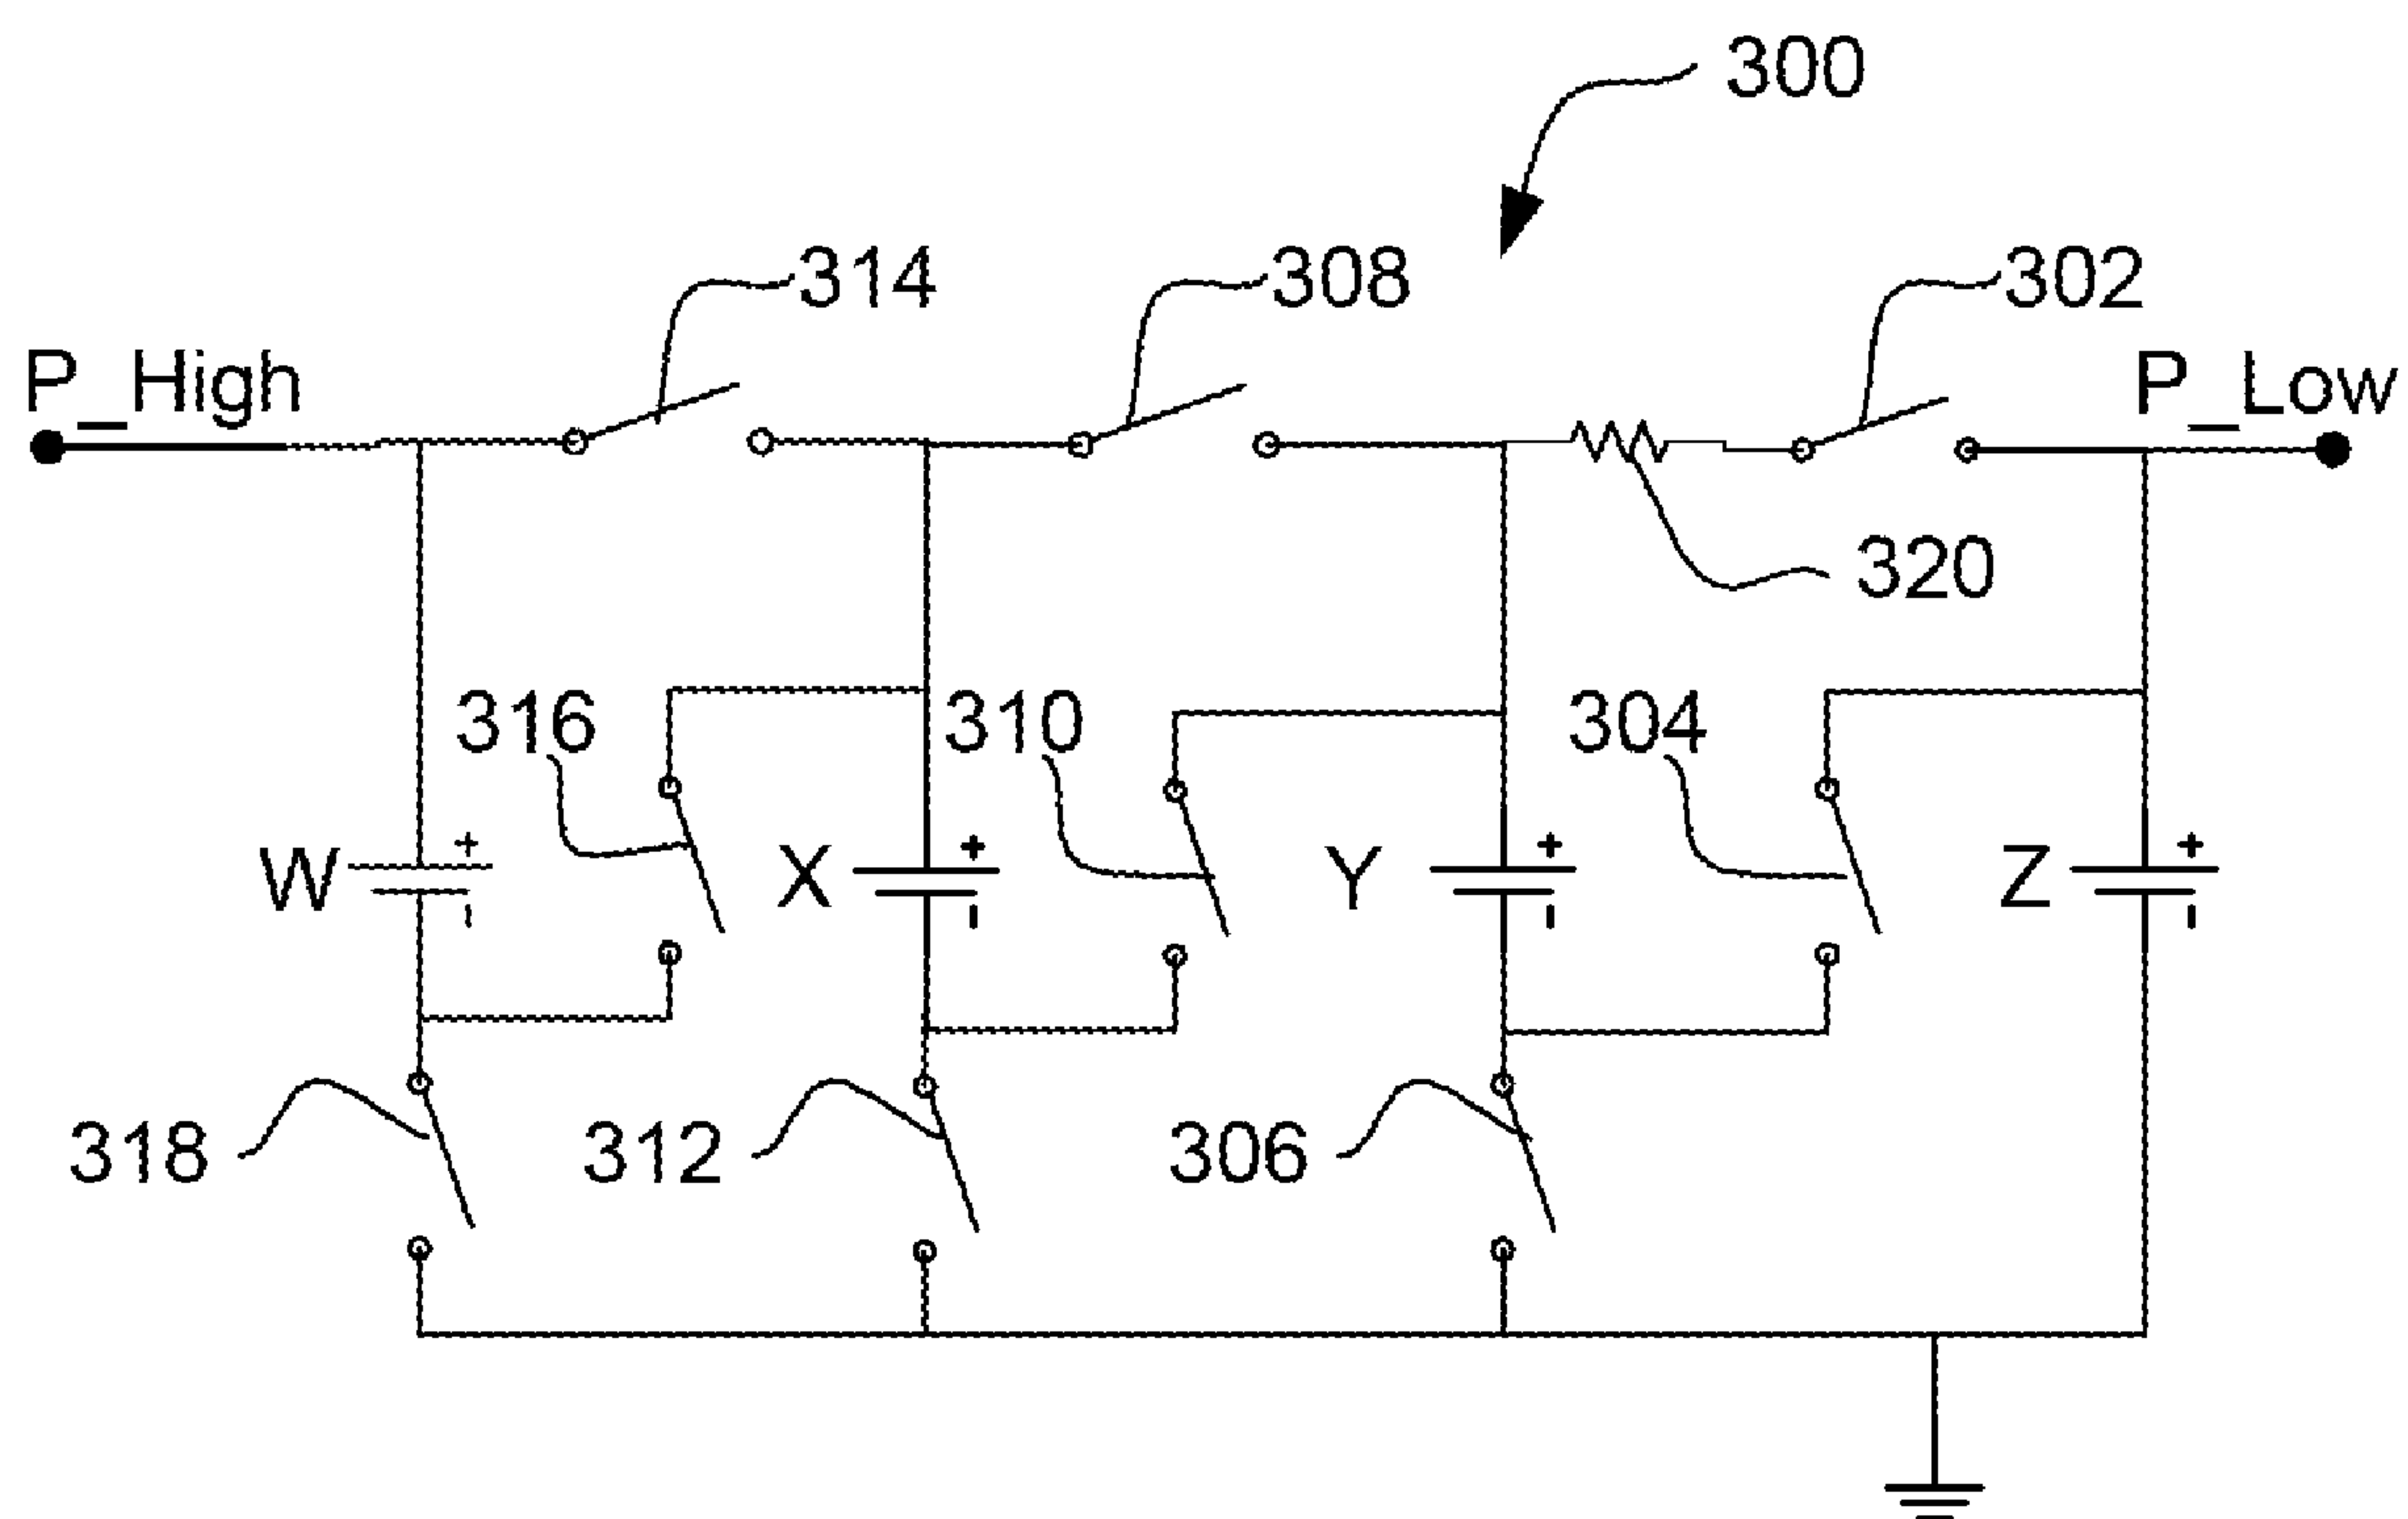

*Figure 6*

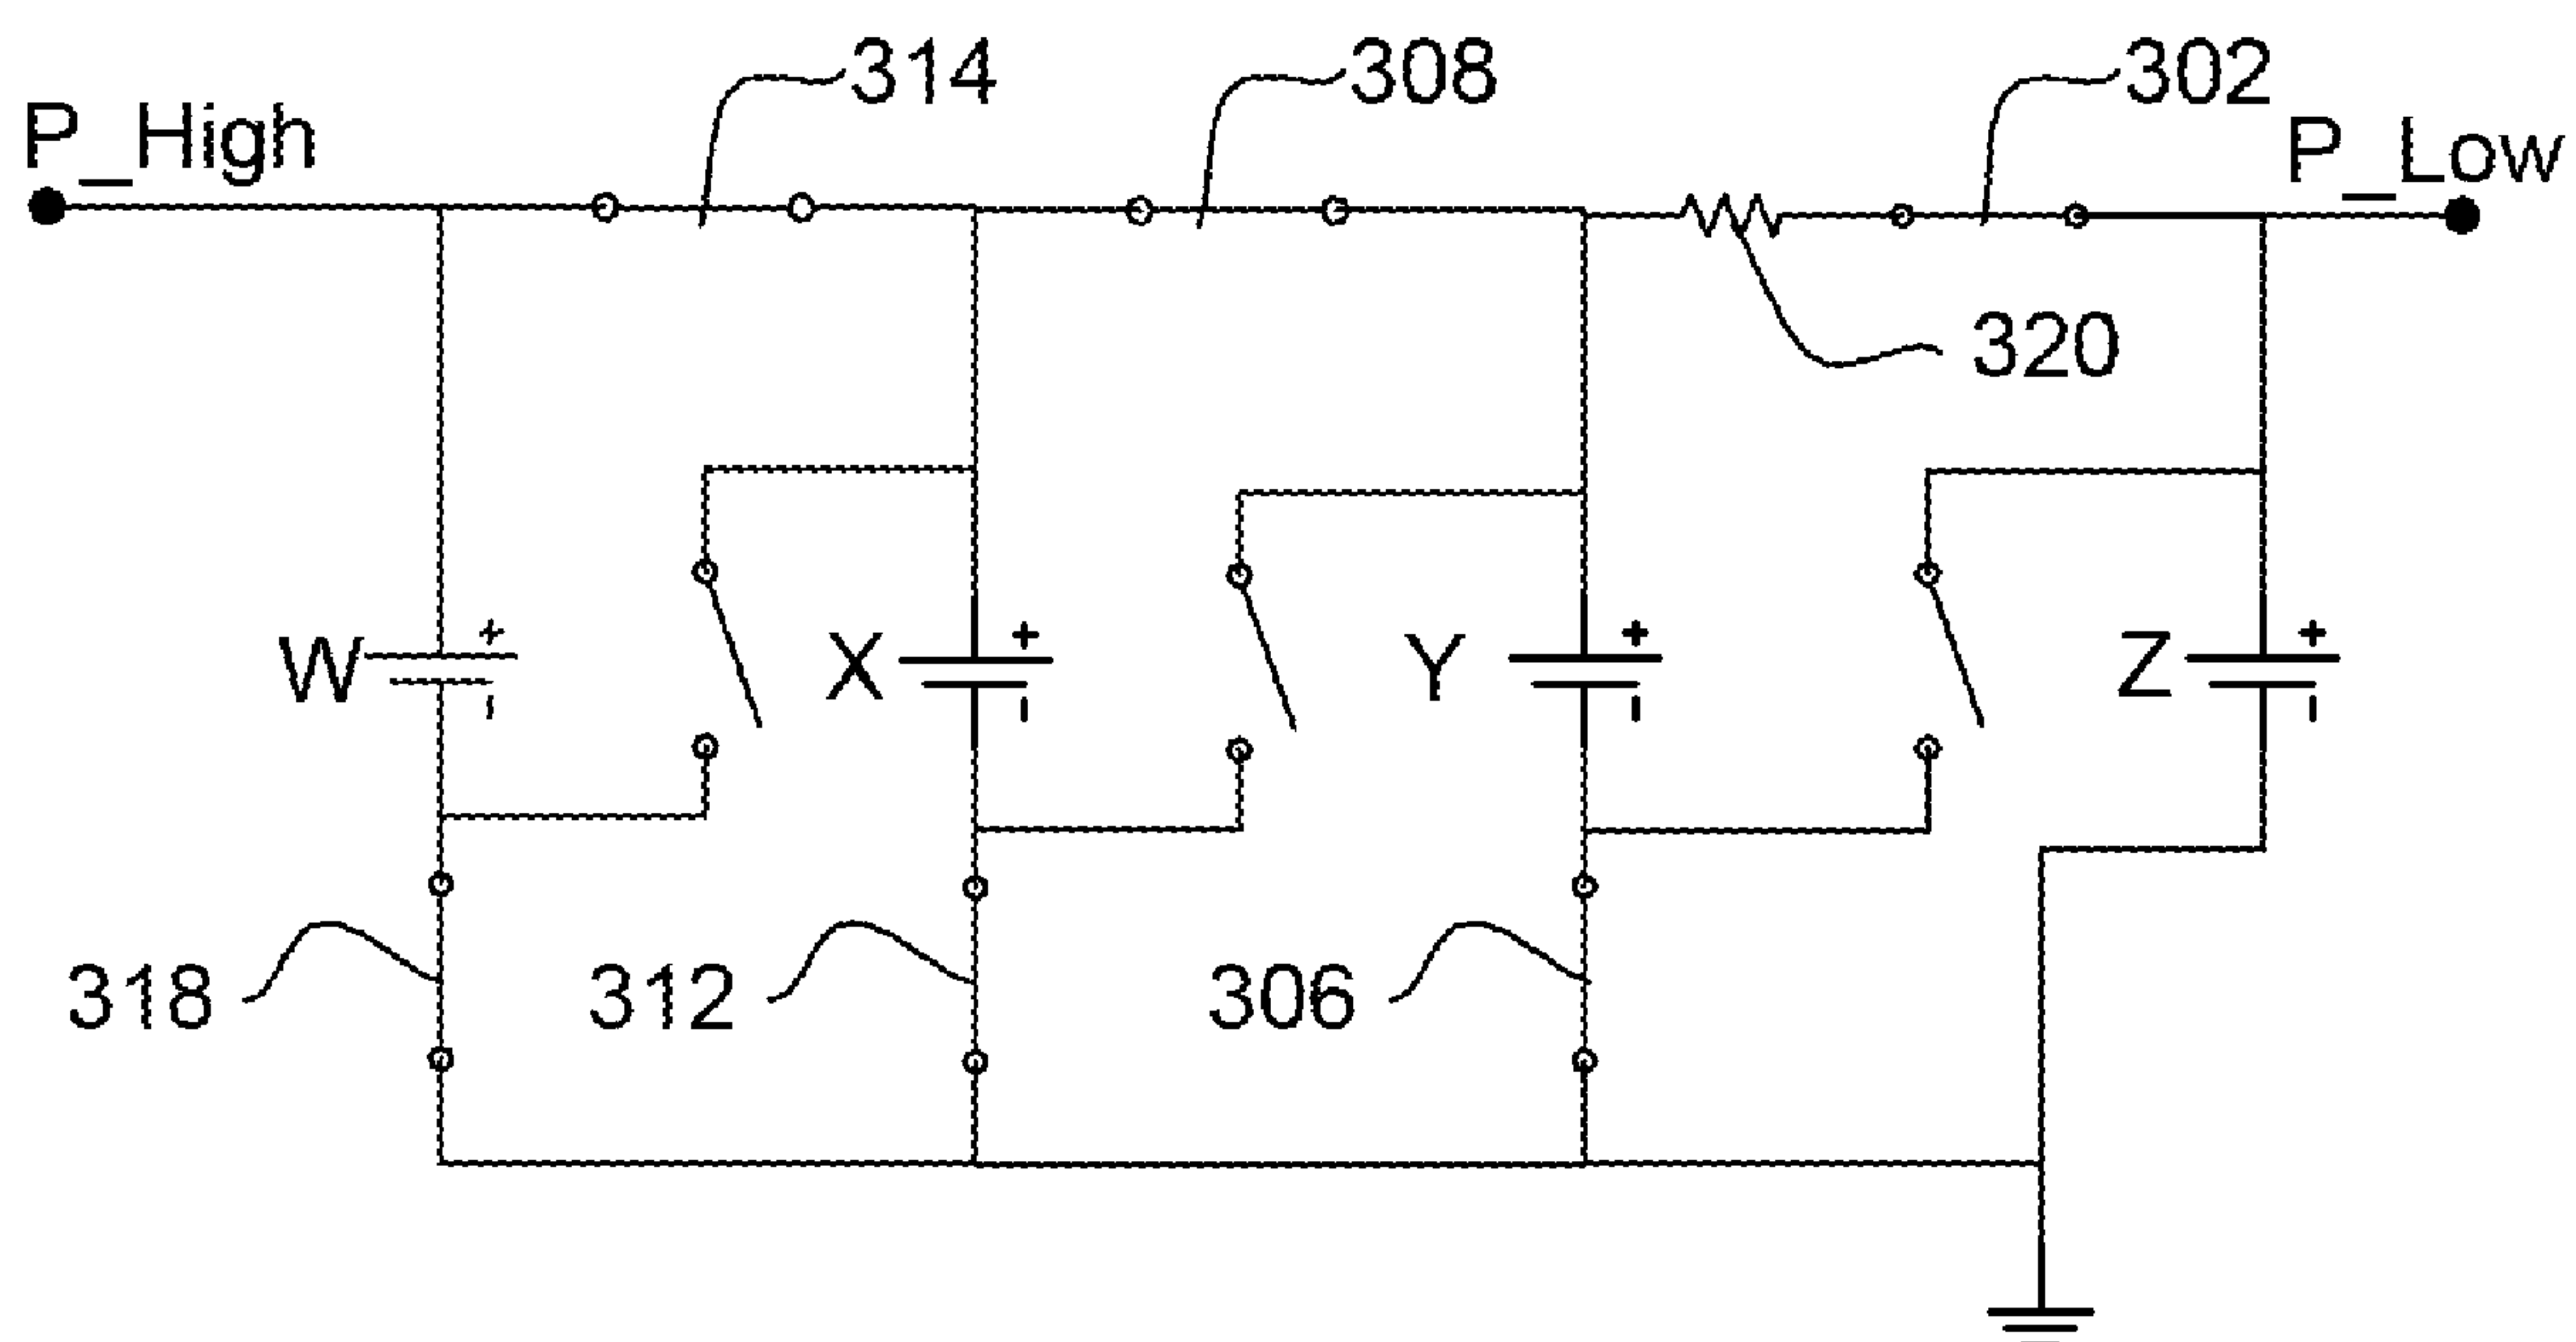

*Figure 7A*

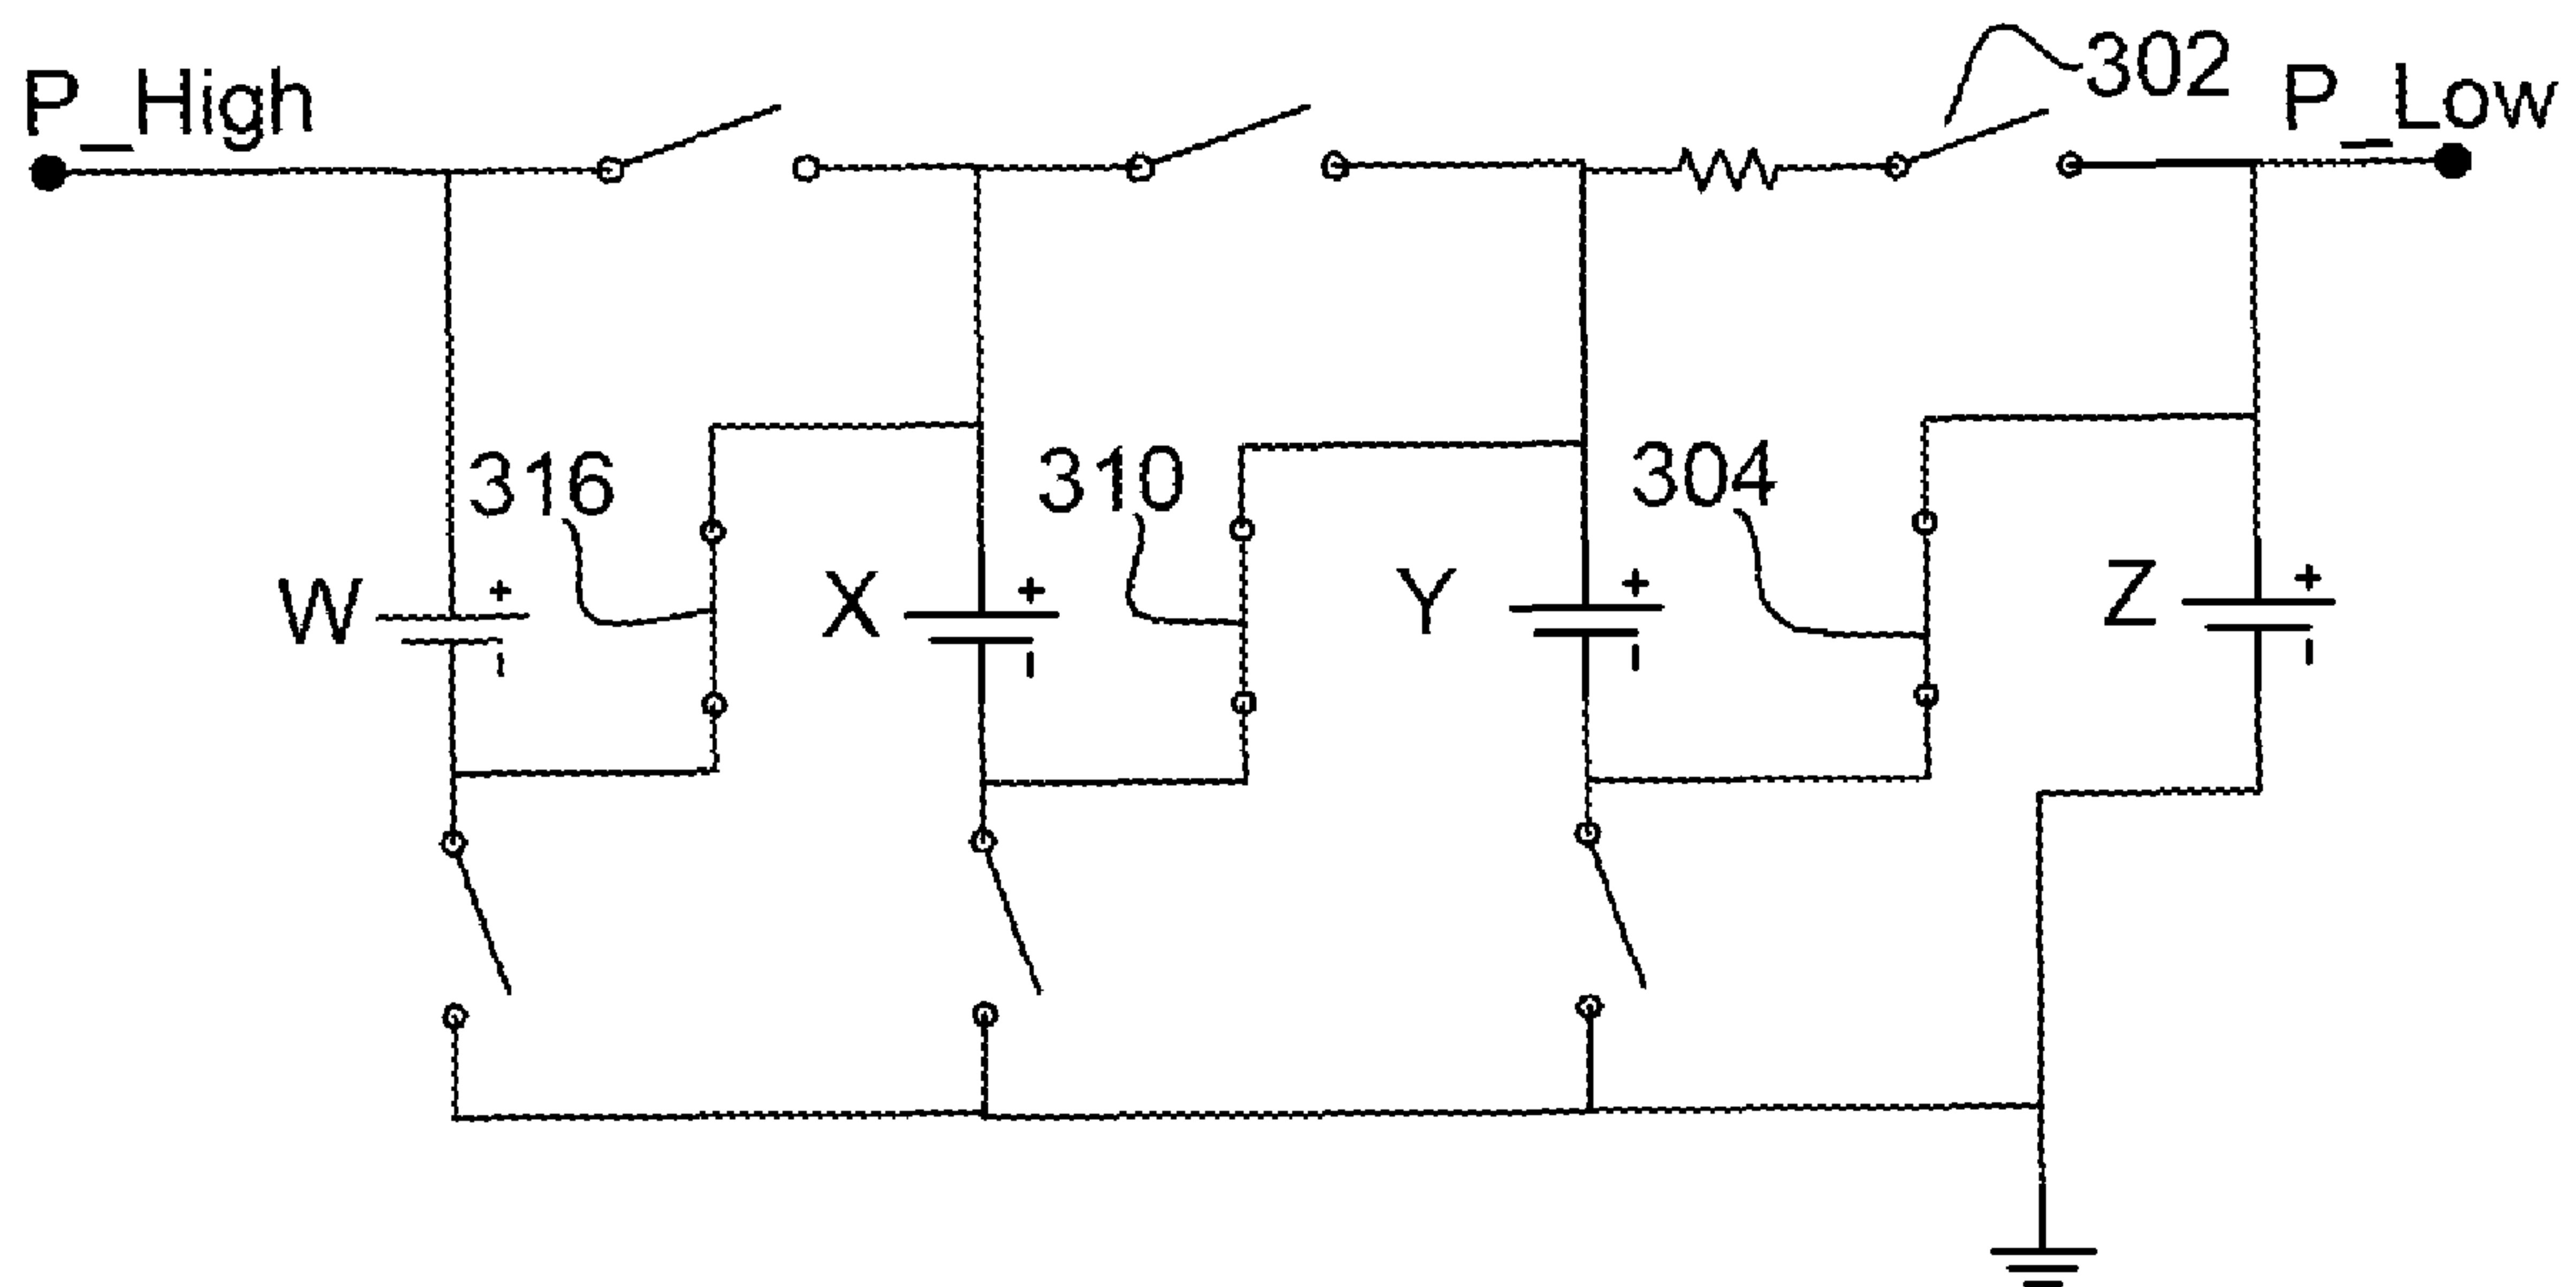

*Figure 7B*

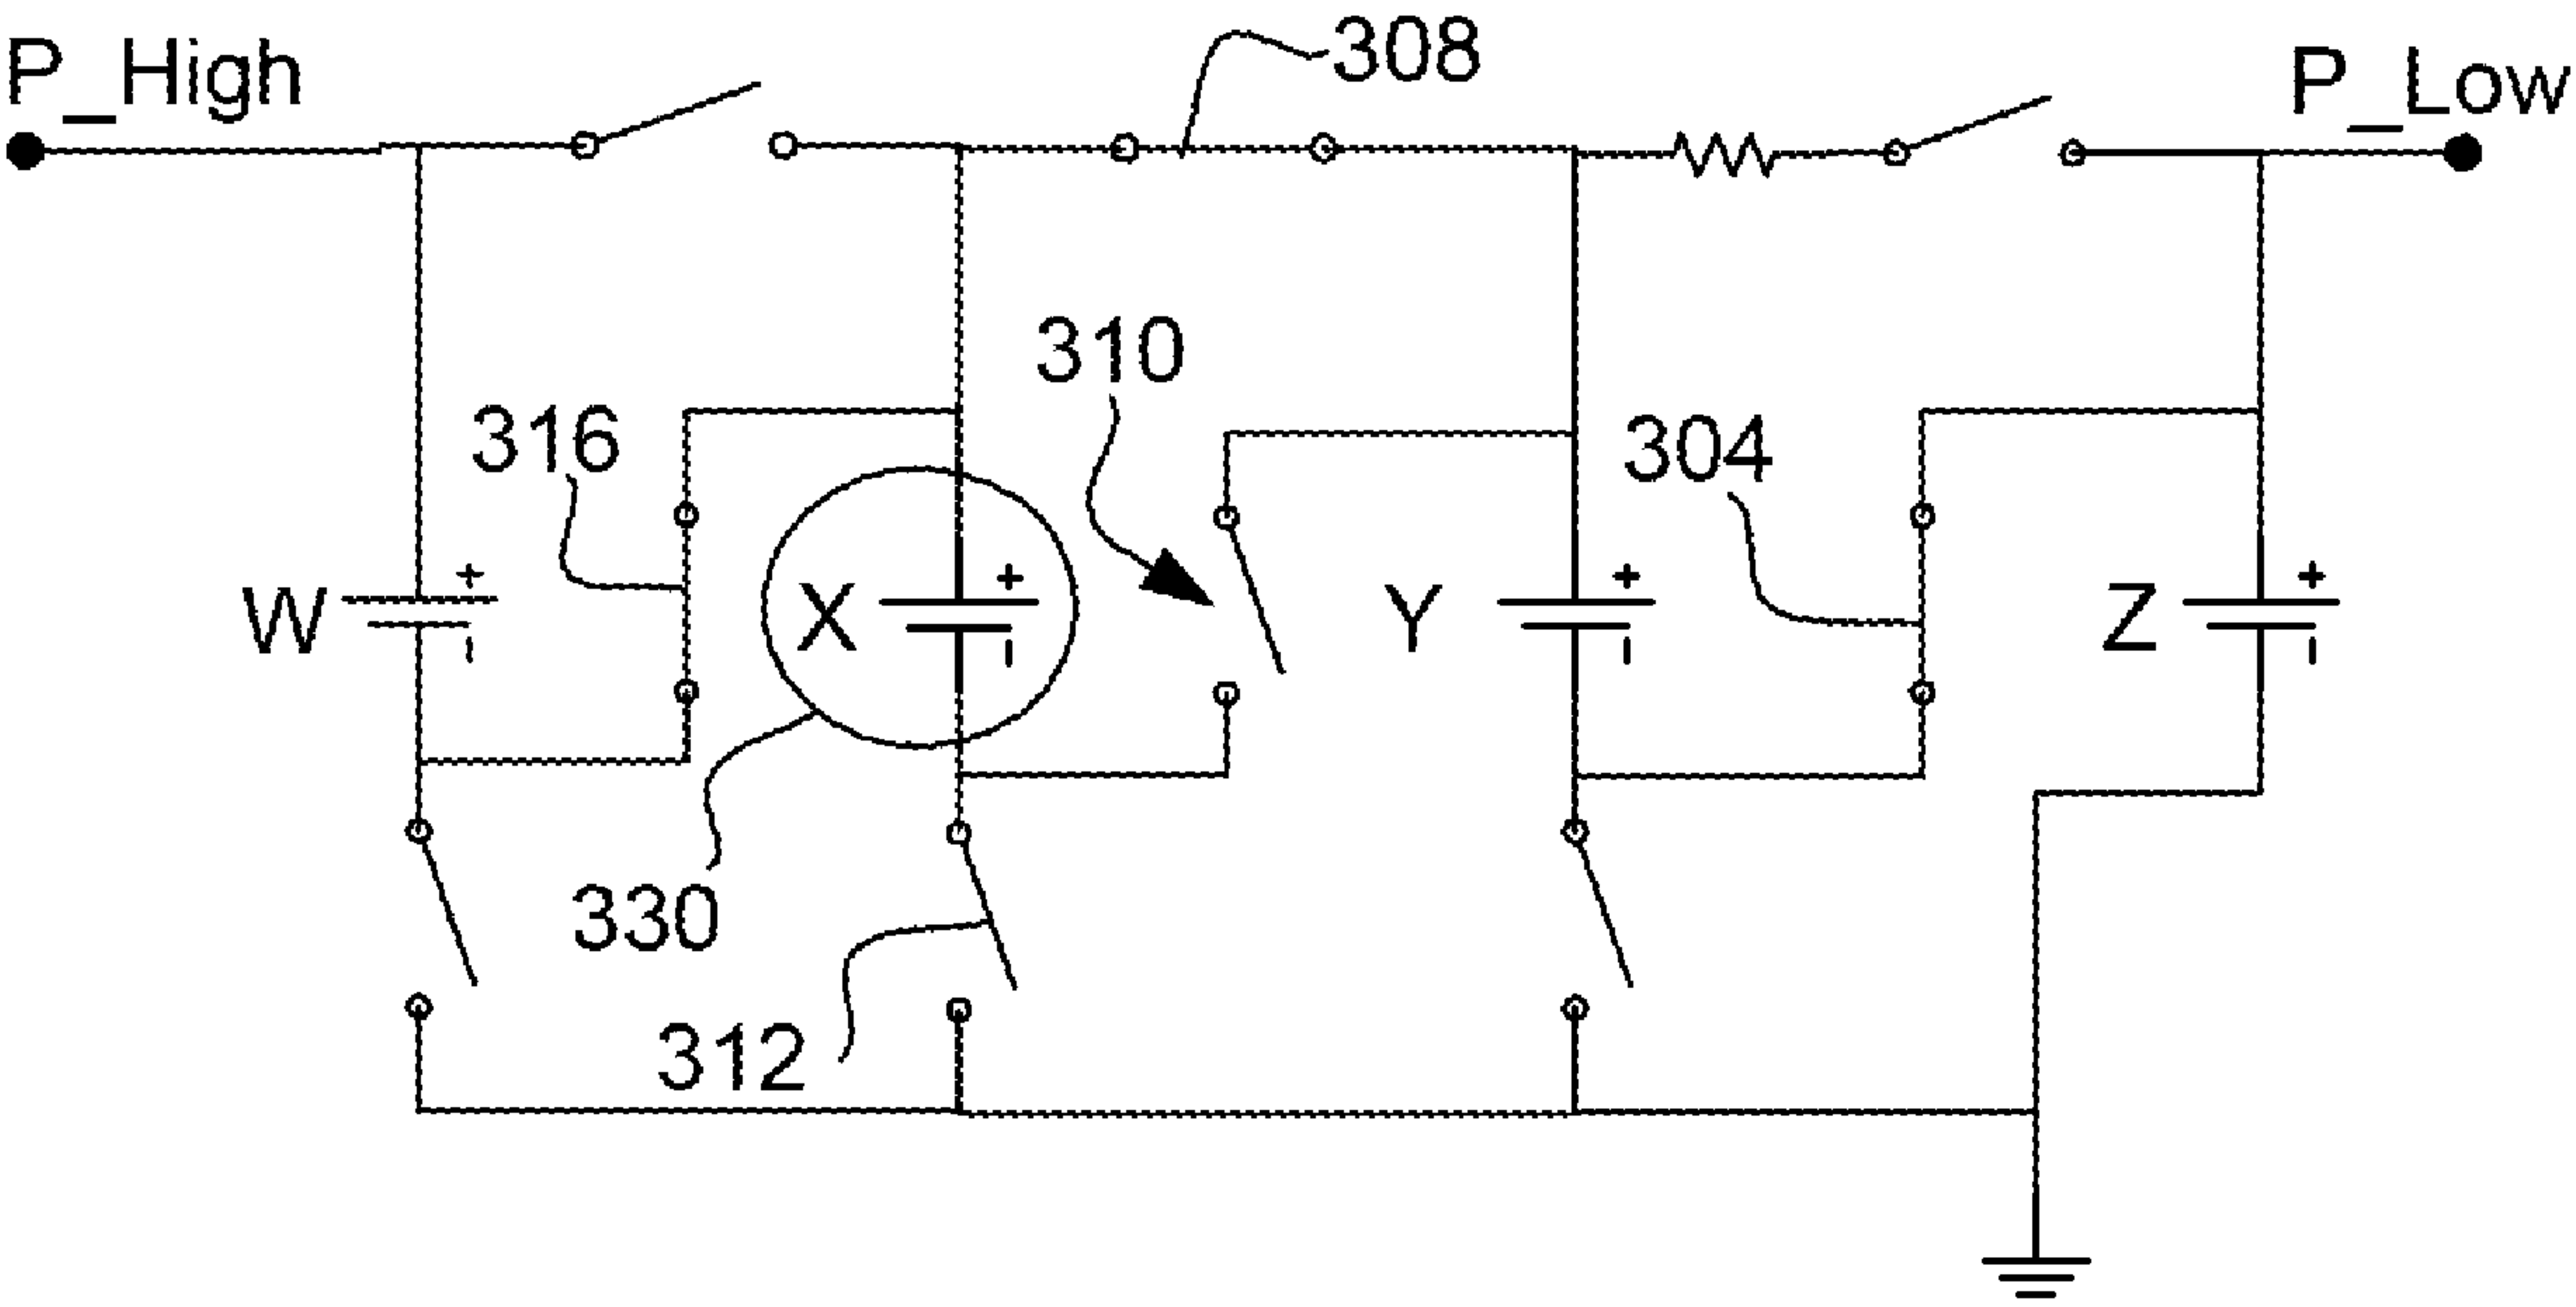


Figure 7C


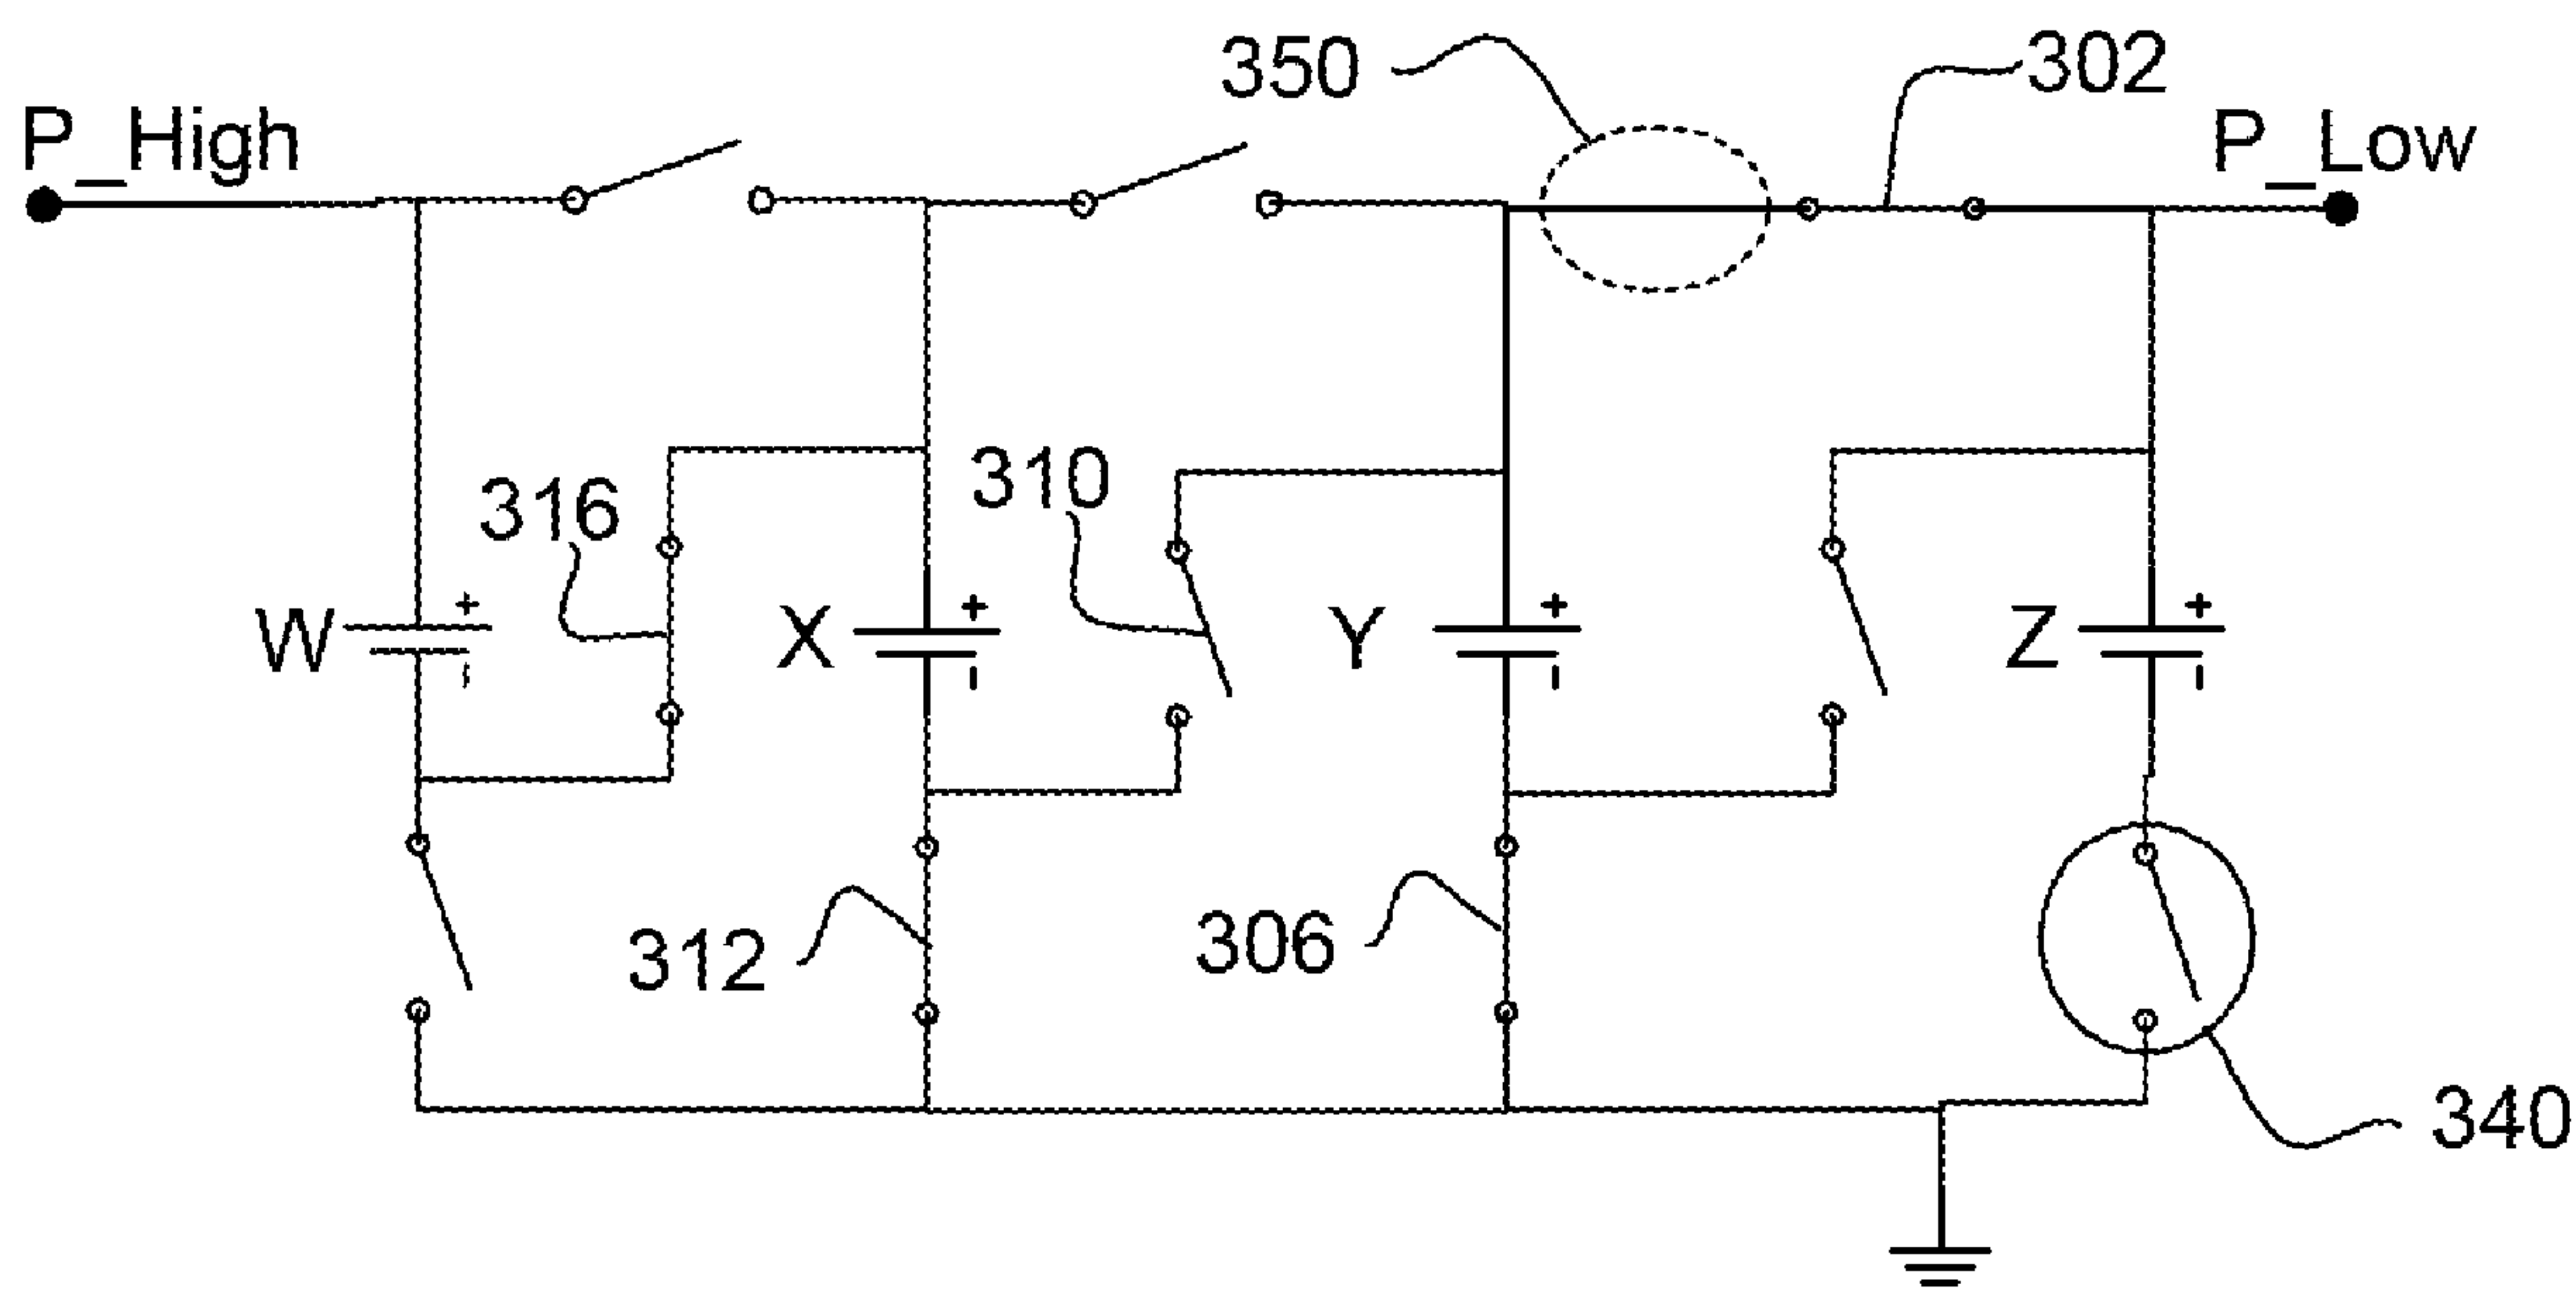


Figure 7D

*Figure 8*

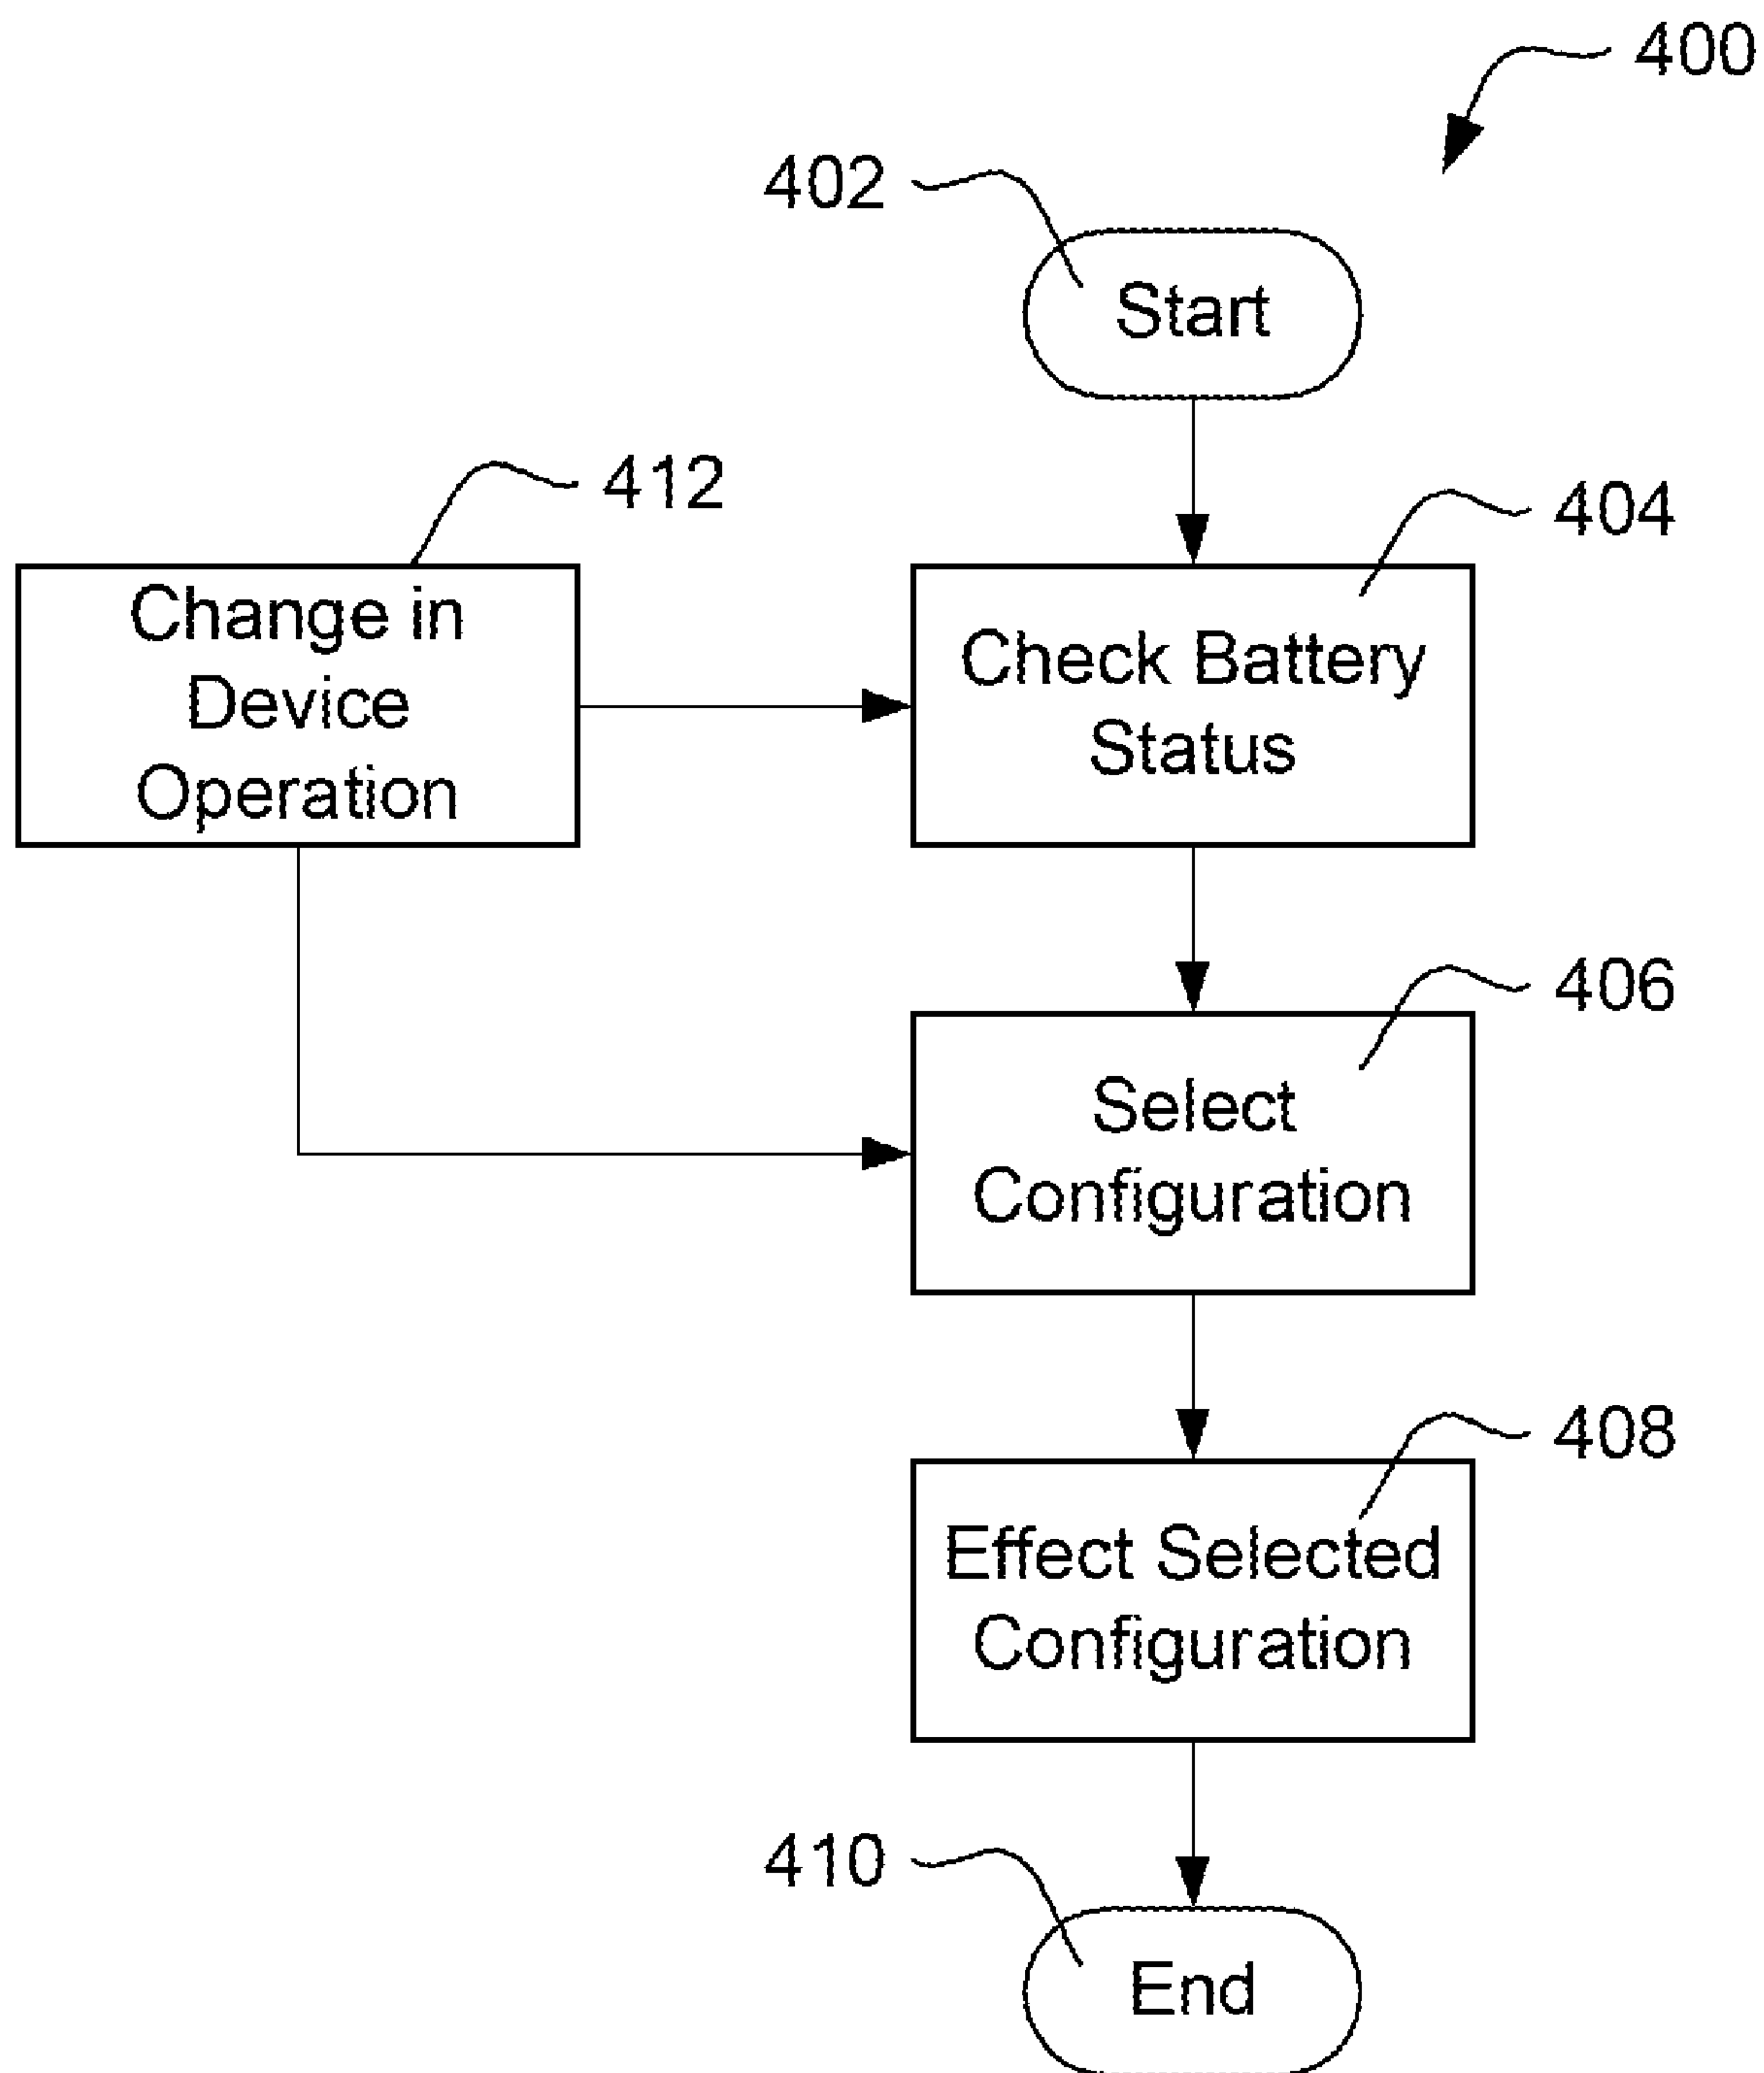

## 1

MULTIPLE BATTERY CONFIGURATIONS IN  
AN IMPLANTABLE MEDICAL DEVICE

## FIELD

The present invention is related to the field of implantable medical devices. More particularly, the present invention relates to electric power supply systems in implantable medical devices.

## BACKGROUND

Some implantable medical device operations require both low-power and high-power functions. An example is an implantable cardioverter-defibrillator (ICD). An ICD monitors cardiac function in a patient using implanted electrodes that capture electrical signals generated by the heart. This monitoring function requires the operation of low power control and analysis circuitry which may include, for example, amplifiers, filters, analog-to-digital converting hardware and/or a microcontroller. The low power circuitry will use currents in the range of microamps at voltages that have been decreasing with improvements in digital and analog circuitry.

In an ICD, monitoring is performed in part to determine whether a malignant arrhythmia is occurring in a patient's heart. If a malignant arrhythmia is identified, high power circuitry is used to build up and then release a large amplitude stimulus to the patient. Such a stimulus may have a voltage of hundreds or even thousands of volts, with total power ranging from less than a Joule up to 80 or more Joules.

A challenge in designing an implantable medical device (IMD) is to find power supply circuitry which can meet the low and high power needs of the device. The simplest approach is to use a single battery. However, challenges arise because available batteries often come in one of two forms: batteries capable of delivering large currents (i.e., high power outputs) but lacking optimal energy density, and batteries having high energy density but which encounter large internal impedances at high currents. One approach could be to provide separate low and high power sources using separate batteries, one having high current output capacity and one having high energy density. However, using separate batteries would cause the device to be disabled as soon as one of the batteries reaches its end-of-life. Alternative solutions are desired.

## SUMMARY

The present invention, in an illustrative embodiment, includes an implantable medical device comprising at least first and second batteries and switching circuitry associated with the first and second batteries. In an illustrative example, a plurality of configurations are provided by the switching circuitry such that, in a first configuration, the batteries operate in parallel with anodes and cathodes coupled together, equalizing voltage output; in a second configuration, the batteries operate in series with the anode of one battery coupled to the cathode of the other battery such that low and high power outputs may be taken from the nodes at each of the anodes; in a third configuration, the batteries are isolated from one another. More than two batteries may be used. Some embodiments include configurations in which one or more batteries may be entirely excluded from operation, if so desired, for example, after it is determined that a battery is near its effective end-of-life. Additional illustrative embodiments include methods associated with such devices. In another embodiment, the configuration of a power circuit in

## 2

an implantable medical device is selected in response to changes in device state or operation.

## BRIEF DESCRIPTION OF THE FIGURES

FIGS. 1A-1B show respective subcutaneous and transvenous implantable cardiac stimulus systems;

FIG. 2 is a functional block diagram for an illustrative implantable medical device;

FIG. 3 is a schematic for an illustrative embodiment;

FIGS. 4A-4C show the illustrative embodiment of FIG. 3 in three configurations;

FIG. 5 is an illustrative embodiment having three batteries;

FIG. 6 is an illustrative embodiment having four batteries;

FIGS. 7A-7C show the illustrative embodiment of FIG. 6 in three configurations; and

FIG. 7D shows an alternative construction and configuration for the embodiment of FIG. 6; and

FIG. 8 is a process flow diagram showing an illustrative method.

## DETAILED DESCRIPTION

The following detailed description should be read with reference to the drawings. The drawings, which are not necessarily to scale, depict illustrative embodiments and are not intended to limit the scope of the invention.

FIGS. 1A-1B, respectively, show subcutaneous and transvenous implanted cardiac stimulus systems relative to a patient's heart. Referring to FIG. 1A, the heart 10 is shown in relation to an implanted, subcutaneous cardiac stimulus system including a canister 12. A lead 14 is secured to canister 12 and includes sensing electrode A 16, a coil electrode 18, and sensing electrode B 20. A can electrode 22 is shown on the canister 12. Other electrode configurations may be used. An alternative subcutaneous system uses a flexible unitary housing rather than a can 12, with or without a lead. Illustrative subcutaneous systems are shown in U.S. Pat. Nos. 6,647,292 and 6,721,597, and the disclosures of these patents are incorporated herein by reference.

A vector for delivering cardiac stimulus is defined between the can electrode 22 and the coil electrode 18. Other vectors for stimulus delivery may be defined depending upon the internal circuitry of the device, different lead designs, and/or the size and shape of electrodes A and B 16, 20, which may also be used for stimulus delivery if so suited. The stimulus vector is illustrated as having two polarities. In addition, although not shown, a number of sensing vectors are defined, for example, using combinations of electrode A 16, electrode B 20, can electrode 22, and/or, if desired, coil electrode 18.

Referring now to FIG. 1B, a transvenous system is shown relative to a patient's heart 30. The transvenous cardiac stimulus system includes a canister 32 connected to a lead 34. The lead 34 resides partly within the patient's vasculature, enters the patient's heart, and includes sensing electrodes A 36 and B 38. Stimulus electrodes are shown at 50, 52. The lead 34 may be anchored into the patient's myocardium. Again, a can electrode 40 is shown on the canister 32. With this system, plural sensing and stimulus delivery vectors may be defined. The embodiment shown includes two stimulus delivery vectors each having two polarities, that is, stimulus vectors between electrodes 50 and 52 and between electrodes 40 and 50. A third stimulus vector may also be defined between electrodes 40 and 52, although this is not shown in the illustration. Other lead and electrode configurations may also be used.



Each of the devices **12**, **32** may further include such components as would be appropriate for communication (such as RF communication, inductive telemetry or other suitable communication linkage) with an external device such as a programmer. To this end, programmers **24** (FIG. 1A) and **42** (FIG. 1B) are also shown. For example, during an implantation procedure, once the implantable device **12**, **32** and leads (if included) are placed, the programmer **24**, **42** may be used to activate the implanted device **12**, **32**, and/or direct/observe diagnostic or operational tests. After implantation, the programmer **24**, **42** may be used to non-invasively determine the status and history of the implanted device. The programmers **24**, **42** in combination with the implanted devices **12**, **32** may also allow annunciation of statistics, errors, history and potential problems to the user/medical practitioner, and may also allow for updating of programming in the implanted devices **12**, **32**.

The systems shown in FIGS. 1A-1B are merely illustrative. The present invention may be embodied in virtually any implantable system. For example, it may be embodied in transvenous or subcutaneous systems such as those shown in FIGS. 1A-1B, as well as hybrid systems combining features of both. Additionally, the present invention may also be embodied in fully intravascular systems modeled on those shown in U.S. Pat. Pub. No. 2006/0224225A1 to Ransbury et al. Although explained in the context of a cardiac stimulus system, the present invention may also be embodied in other implantable medical systems directed toward other portions of the anatomy.

FIG. 2 is a functional block diagram for an illustrative implantable cardiac stimulus device. In the illustrative example, operational circuitry for an implantable cardiac stimulus device is shown at **100**, a patient is shown both at **102a** and **102b**. It should be understood that this is the same patient in both instances **102a**, **102b**, but the coupling electrodes may be different for each. For example, shock delivery electrodes may be separate or different from sensing electrodes, although this need not always be the case.

The operational circuitry includes a control block **104**, which may take any suitable or conventional form. Microcontrollers are one class of device that may be used in control block **104**, although in addition to or as a replacement for a microcontroller, there may be various logic and other devices or subcircuits. The control block **104** may access a memory **108**, which may take various forms including RAM, ROM, Flash memory, or any other suitable form (optical, electrical, magnetic, etc.) for temporarily or permanently storing information and/or instruction sets. The control block **104** is configured and connected to other circuitry within the device such that it can direct operations associated with methods of practicing some illustrative embodiments of the present invention. A battery block **106** is also shown. The battery block **106** is more fully explained below.

The operational circuitry **100** may also include telemetry **110**, which may include such drivers, mixers, antenna(s), amplifiers and the like as are known for use in communications circuitry. The telemetry **110** is used to communicate with a programmer, such as programmers **24**, **42** shown in FIGS. 1A-1B.

Signal capture block **112** includes amplifying and filtering circuitry which may take any form suitable for use in an implantable cardiac stimulus device for observing cardiac function. Signal capture block **112** may also include sampling and analog-to-digital devices, as well as local registers, memory or the like for temporarily storing captured information.

Generally speaking, the control block **104** uses the signal capture block **112** to capture data from the patient **102a**. In response to instructions from telemetry **110** and/or instructions or data stored in memory **108**, the control block **104** may analyze data from the signal capture block **112** to determine whether the patient **102a/b** is in need of stimulus. If so, the control block **104** calls on the charger **114** to charge energy storage **116**, which may include one or more capacitors in any suitable configuration. As is known to those of skill in the art, the charger **114** is used to step up the voltage from the battery **106** (typically less than 10 volts) to a higher level (up to several hundred or even several thousand volts) for use in cardioversion or defibrillation. In order to achieve sufficient energy storage, the charger **114** typically draws significantly larger currents than other portions of the operational circuitry **100**.

The control block **104** and/or the charger **114** may monitor the voltage level on the energy storage **116** during charging to determine whether and when sufficient stimulus energy has been stored. Once enough energy is stored at energy storage **116** for stimulus delivery, the control block **104** manipulates output circuitry **118**, which may include, for example, a plurality of switches and/or an H-bridge configuration, in order to deliver the stored energy to the patient **102b**. An H-bridge is shown, for example, in U.S. Pat. Nos. 6,865,417 and 6,952,608. In other medical devices, there may be output circuitry, such as transducers (such as sonic drivers for phoresis delivery of a drug), pumps, etc., that take the place of the illustrative subcircuits shown at **114**, **116** and **118** in FIG. 2.

In the illustration, the battery block **106** is shown as providing a Low Power portion **106A**, which powers the control block **104**, telemetry **110**, and signal capture block **112**. For illustrative purposes, not all connections are shown. The battery block **106** also includes a High Power portion **106B**, which is used to power a charger **114**.

In an illustrative example, the control block **104** can manipulate the duration and format of the applied stimulus by controlling the output circuitry **118**, for example, controlling whether the applied waveform is monophasic or biphasic, and also controlling the amplitude and polarity. It is typical for the amplitude of the applied voltage to drop during its application as the energy storage **116** (typically a bank of capacitors) discharges energy. The change in output amplitude during an applied pulse is sometimes referred to as "tilt," a ratio of the final voltage to the initial voltage. Constant current stimuli may also be applied.

FIG. 3 is a schematic for an illustrative embodiment of a power system. The illustrative embodiment includes a high output battery Bh, shown at **200**, and a low output battery B1, shown at **202**. The batteries **200**, **202** are coupled to high and low outputs shown, respectively, at P\_High and P\_Low, which are taken with respect to a common ground, as shown. Three switches **210**, **212**, and **214** selectively couple the batteries **200**, **202** to the outputs, ground, and each other. An optional attenuating resistor is shown at **220**.

The switches **210**, **212**, **214** may take any suitable form, including for example, MOSFET, JFET and/or BJT electrical devices. Other devices, such as relays and/or silicon controlled rectifiers, may also be used. It should be understood that control wires for these switches **210**, **212**, **214** have been omitted from the Figures for simplicity.

As shown, switch **212** selectively couples the positive terminal + of the low output battery B1 **202** to the negative terminal - of the high output battery Bh **200**. Switch **214** selectively couples the negative terminal of the high output battery Bh **200** to ground. The positive terminal of the high output battery Bh **200** is directly coupled to a P\_High output



## 5

of the battery subcircuit, while the positive terminal of the low output battery **202** is directly coupled to a P\_Low output of the battery subcircuit. The operation of the switches to provide multiple configurations is further illustrated below by reference to FIGS. 4A-4C.

In an illustrative example, P\_High is used to power high current portions of the implantable device circuitry, and P\_Low is used to power low current portions of the implantable device circuitry. For example, in an ICD, P\_High is used to power charging circuitry that quickly stores up energy on power capacitors for delivering as a defibrillation pulse, while P\_Low can power the control circuitry. In another illustrative example, P\_High is element **106B** in FIG. 2, while P\_Low is element **106A** in FIG. 2.

In an illustrative example, the batteries **200** and **202** may differ in chemistry and/or structure such that each has distinct characteristics. For example, the low output battery **202** may be a battery having relatively higher internal impedance than the high output battery **200**, but higher energy density, making the low output battery **202** well suited to providing power for long-term operation of control and monitoring circuitry, while the high output battery **200**, with the lower internal impedance, would be better suited to powering high current applications such as charging a high power capacitor for use in delivering large stimulus. In an alternative embodiment, the batteries **200**, **202** may be of the same construction as one another.

FIGS. 4A-4C show the illustrative embodiment of FIG. 3 in three configurations. In FIG. 4A, switch **212** is closed, while switches **210** and **214** are open. This couples the positive terminal + of the low output battery **202** to the negative terminal – of the high output battery **200**, placing the batteries **200**, **202** in series. The output of the series is at P\_High, and an output is taken between the batteries **200**, **202**, as P\_Low. The illustration to the right of the drawing shows this simplified circuit. The voltage at P\_High will be the sum of the voltages across the batteries **200**, **202**, which in turn reduces the equivalent current draw at P\_High during high power output, since less current is drawn to produce the same power output at this summed voltage.

In FIG. 4B, switch **212** is left open, while switches **214** and **210** are closed. As shown to the right, this configuration places P\_High and P\_Low in parallel connection with one another across the optional resistor **220**, which may be omitted if desired. This configuration allows either battery **200**, **202** to make up for a deficiency of the other battery. The optional resistor **220** can be used to prevent shorting of one battery **200/202** to the other **202/200**, for example, if the batteries **200**, **202** have different output voltages. Alternatively, the optional resistor **220** may be omitted to prevent attenuation of energy within the circuit.

In an alternative configuration, an additional switch may be placed between the negative terminal of the low output battery **202** and ground. This switch may be opened to remove the low output battery **202** from the circuit entirely, which may be desired if the low output battery **202** reaches or nears its end-of-life. Then all circuitry would be powered from the other battery. Conversely, the configuration of FIG. 4B may be modified to open switch **214**, removing the high output battery **200** from the circuit entirely, since the negative terminal of the high output battery **200** would then be left floating. This would allow the low output battery **202** to power the entire device in the event that the high output battery **200** reaches or nears its end-of-life. In some embodiments, each battery may be individually tested to determine whether

## 6

either is at or near its end-of-life, for example, by monitoring changes in internal impedance, loaded voltage, or open circuit voltage.

In some illustrative examples, battery status may be measured by one or more of the following methods. An illustrative method may include coupling a battery output to a high impedance input to an analog-to-digital converter to check open circuit voltage. Another illustrative method may include measuring a voltage across a resistor, to check loaded voltage of the battery. If both such measurements are taken, yielding  $V_{Open}$  and  $V_{Loaded}$ , and the resistor size is known, the internal impedance of a battery may be identified by noting that the resistor and the internal resistance of the battery form a voltage divider, with:

$$V_{Open} = V_{Loaded} \times \frac{R_{Load} + R_{Internal}}{R_{Load}}$$

Solving for the internal resistance:

$$R_{Internal} = R_{Load} \times \left( \frac{V_{Open}}{V_{Loaded}} - 1 \right)$$

Another method of measuring battery status is disclosed in copending U.S. patent application Ser. No. 11/487,103, entitled END OF LIFE BATTERY TESTING IN AN IMPLANTABLE MEDICAL DEVICE, filed on Jul. 14, 2006, the disclosure of which is incorporated herein by reference. Any of these methods and metrics (open circuit voltage, loaded voltage, and internal impedance or resistance) may be used to determine battery status and estimate the end-of-life (EOL) for a battery. Additional methods, devices and sub-circuits for testing any of these metrics, or other metrics indicating battery status, are known in the art as well. Battery status may be annunciated to an associated programmer when queried or whenever a battery nears EOL. If EOL approaches or occurs, the device may notify an implantee, as is known in the art.

In yet another embodiment, a switch is supplied between the positive terminal of the low output battery **202** and the P\_Low output, with the configuration of FIG. 4A being used. In this manner, the two batteries **200**, **202** can be used in series to supply power for both the P\_High and P\_Low outputs; this may be desired when either or both batteries are near end of life. While it is likely best that a patient seek medical attention, likely including explant and replacement of the device, when end of life for either or both batteries is near, the device itself, as implanted, can be configured to maximize the available battery power even if the patient delays in obtaining medical attention.

FIG. 4C demonstrates yet another configuration. Here, switches **210** and **212** are left open, isolating the batteries from one another. The result is that the P\_High output is provided exclusively by the high output battery **200**, and the P\_Low output is provided exclusively by the low output battery **202**.

Usage of these configurations may be programmed into a device. The configuration of FIG. 4C may be used, in this example, as a default or standard configuration during ordinary operation of an implantable medical device (IMD) such as an ICD. If the ICD is also equipped to provide a pacing output, the configuration of FIG. 4C may be used during pacing, with P\_High and hence only the high output battery **200** used to provide pacing output energy, while P\_Low and



hence only the low output battery **202** used to power associated control circuitry. If a defibrillation or cardioversion stimulus is used, either the configuration of FIG. **4C** or the configuration of FIG. **4A** may be used. In one example, the power supply switches are adjusted to the configuration of FIG. **4A** in the event that a high voltage pulse charge fails to build on associated capacitors within a predetermined period of time. In another example, the configuration of FIG. **4A** is used when multiple large amplitude stimuli are needed within a short period of time. In yet another example, an ICD is configured to provide defibrillation pulses having increasing amplitudes (i.e., 5 Joules, 10 Joules, 15 Joules, etc.), and the configuration of FIG. **4C** is used for lesser amplitudes, while the configuration of FIG. **4A** is used for greater amplitudes. The configuration of FIG. **4B** may be used near the end of life of the low output battery **202**.

FIG. **5** is an illustrative embodiment of a power system **250** having three batteries. In the illustrative embodiment, batteries **R**, **S**, and **T** are shown coupled together with a plurality of switches **252**, **254**, **256**, **258**, **260**, **262**. It can be seen, when compared to FIG. **3**, that the embodiment of FIG. **5** is similar except that a module of battery **R** and switches **258**, **260**, **262** has been added.

The following chart is illustrative of operation:

Configuration	252	254	256	258	260	262	P_High	P_Low
1	○	X	○	○	X	○	R + S + T	T
2	X	○	X	X	○	X	R = S = T	R = S = T
3	X	○	○	X	○	X	R + T	T
4	○	X	○	X	○	○	S + T	T
5	○	○	X	○	X	○	R + S	T

Additional configurations can be added as well. Configuration 1 allows all three batteries to contribute during a high power output time period. Configuration 2 allows each battery to contribute to high and low power output, for example, to compensate for one of the batteries being at or near its end-of-life. Configuration 3 allows a battery, in this case, battery **S**, to be isolated, while configuration 4 allows a different battery, in this case, battery **R**, to be isolated. Configuration 5 separates the functions of the batteries completely such that two batteries are dedicated to only high power output **P\_High** while the third battery is dedicated to only the low power output **P\_Low**.

Those of skill in the art will recognize that the pattern and configuration in FIG. **5** can be expanded using  $3(N-1)$  switches to couple **N** batteries together. Those of skill in the art will also recognize that an additional switch may be provided at one of locations **270**, **272** to allow isolation of battery **T** in a manner analogous to configurations 3 and 4 shown above. An example includes another switch at location **272**: switches **256** and **260** would be closed such that  $P_{High} = S + R$ , and switch **252** is closed such that  $P_{Low} = S$ , while switches **254**, **258**, **262** and **272** are opened, with switches **254** and **272** isolating battery **T**, and switches **258** and **262** being opened to allow series operation of batteries **S** and **R** for output **P\_High**.

FIG. **6** is an illustrative embodiment of a power system having four batteries. The embodiment in FIG. **6** includes yet another "module" comprising battery **W** and switches **314**, **316**, **318**, as compared to FIG. **5**. Batteries **W**, **X**, **Y** and **Z** are shown and coupled together. Switches **304**, **310** and **316** selectively couple battery pairs in series with positive terminals

nals coupled to negative terminals for battery pairs **Z/Y**, **Y/X**, and **X/W**, respectively. Switches **306**, **312**, **318** selectively couple the negative terminals of batteries **Y**, **X** and **W**, respectively, to ground. Switches **302**, **308** and **314** selectively couple positive terminals of pairs of batteries together, with switch **302** between batteries **Z/Y**, switch **308** between batteries **Y/X**, and switch **314** between batteries **X/W**. Again, an optional resistor is shown at **320**. The interconnections of the batteries **W**, **X**, **Y**, **Z** and switches **302**, **304**, **306**, **308**, **310**, **312**, **314**, **316** and **318** form a power system.

FIGS. **7A-7C** show the illustrative embodiment of FIG. **6** in three configurations. In FIG. **7A**, all of the batteries are connected in parallel with one another by having switches **302**, **306**, **308**, **312**, **314** and **318** closed. In FIG. **7B**, **P\_Low** is taken from battery **Z** only by opening switch **302**, and the **P\_High** is taken from the series combination of batteries **W**, **X**, **Y**, and **Z** by closing switches **304**, **310** and **316**, while leaving other switches open, as shown. FIG. **7C** shows a configuration in which one battery (battery **X**) is excluded from the circuit as indicated at **330**, which may be necessary if one of the batteries becomes depleted faster than other batteries; alternatively, this may simply be a configuration deliberately chosen for other design purposes. Battery **X** is excluded by closing switches **304**, **308** and **316** and opening switches **310**, **312**, thereby routing current around the excluded battery **X**.

FIG. **7D** shows an alternative construction and configuration for the embodiment of FIG. **6**. This construction includes an additional switch **340** in series with battery **Z** and located between the negative terminal of battery **Z** and ground, and the otherwise optional resistor is omitted as indicated at **350**. In this configuration, opening switch **340** allows battery **Z** to be excluded from the circuit. In the configuration shown, **P\_Low** is powered by battery **Y** alone, while **P\_High** is powered by batteries **W** and **X** in series with one another by closing switches **312** and **316**, while the other switches remain open. The additional switch may be included in other configurations shown herein such that the number of switches in each would then be  $3N-2$  for **N** batteries.

In an illustrative example, battery **Z** may be a battery used by default to power **P\_Low** (for example, battery **Z** may be of different chemistry or construction than batteries **W**, **X** and **Y**). In this example, battery **Z** may near or reach end-of-life well before the other batteries if the device is implanted for prophylactic purposes in a patient who rarely needs high power therapy, as may happen if a high risk patient eliminates risk factors by changes to habits, diet, exercise and/or medication and sees substantial improvement. In this scenario, the remaining batteries may be reconfigured as shown to provide a low power output **P\_Low** without continued reliance on the end-of-life battery. As an alternative to that shown in FIG. **7D**, switch **310** may be closed while switch **312** is opened, allowing the **P\_High** output to be generated by the series combination of all three of batteries **W**, **X** and **Y**.

In an illustrative example, at least one of the batteries is coupled to the **P\_Low** node in series with a switching device that is "closed" when no voltage is applied. For example, switch **340** may be a depletion-type MOSFET, which turns off when a voltage is applied to its control terminal. This may simplify device turn-on, since at least one battery is coupled between **P\_Low** and ground without any voltage output from a control terminal to the depletion-type MOSFET.

FIG. **8** is a process flow diagram showing an illustrative method. The method **400** may begin from a start block **402**, which will in some embodiments be initiated at intervals, for example, daily, weekly or at lesser or greater intervals. The method **400** may also be initiated in response to a query



during a session in which communication is established between an implanted device and a programmer.

First, battery status is checked, as indicated at **404**. In some embodiments, all batteries in the system may be checked during step **404**. Alternatively, only batteries which are known to have produced currents during operation may be tested, for example, in an ICD, it is possible for monitoring of cardiac activity, which is a relatively low power function of the device, to occur for a great period of time without any stimuli being delivered to an implant recipient. In this instance, the method may perform a battery status check on only the battery(ies) that are powering the low power functions. In yet another embodiment, all batteries are checked to monitor for conditions that indicate device or battery malfunction. Although not shown, in response to step **404**, a flag or other stored value may be set by the implanted device to indicate the battery status and/or if one or more batteries are at or near end-of-life. If and when communication is established with an external programmer, such flags or values may be annunciated.

From step **404**, the device continues to step **406**, in which a battery configuration is selected. Next, the selected battery configuration is effected, as shown at **408**, by opening and/or closing appropriate switches in the power supply circuit. The method then ends, as shown at **410**. In an illustrative example, an indicator of the configuration in use can be stored and this indicator is annunciated during communication with an external programmer.

In addition to periodic starting at **402**, in some embodiments, a change in device operation **412** may cause initiation of method **400**. This may occur, for example, when it is determined that a high power output is needed from the power supply circuit, for example, when a malignant arrhythmia is detected by an ICD and stimulus is needed, or when a bradyarrhythmia is detected by a pacemaker and pacing is indicated, or when stimulus of another portion of patient anatomy, such as parts of the nervous system, is needed. In one example of an ICD, the change in device operation may also occur during operation if multiple stimuli are delivered at increasing amplitudes. The change in device operation **412** may occur if a time-out occurs during charging of a high power capacitor in an ICD as may happen if the previously selected configuration fails to provide adequate current/power to charge the high power capacitor quickly. In another example, the implanted medical device may be a drug delivery device having output circuitry for delivering a drug to a patient, or having a pump that requires operation, and the decision to deliver the drug represents a change in device operation. Similarly, block **412** may be an indication that use of the high power output has ended, such that a different configuration adapted for delivery of only low power output may be adopted.

Initiation of method **402** from block **412** may go to either block **404** or block **406**. For example, if the method is embodied in an ICD and a high power stimulus is to be delivered to prevent sudden cardiac death, a new configuration **406** may be selected without re-checking battery status, in order to reduce delay between the decision to deliver stimulus and actual stimulus delivery. Alternatively, in a device such as an insulin pump, a delay of a few seconds to allow battery status to be checked in step **404** may be acceptable.

In the example of an ICD, if the change in device operation occurs due to a time-out occurring during high power capacitor charging, a check of battery status **404** may be performed to determine why the time-out occurred—and, if one or more batteries is at or near end-of-life, to remove the offending battery from the high power output circuit. For example, a

battery at or near its end-of-life may undergo an increase in internal impedance, which may introduce a time constant into the charging circuitry that prevents fast charging. If such a battery is placed in series with the high power output, one “dead” battery in series with one or more non-depleted batteries can prevent the other batteries from successful charging.

In an illustrative embodiment, the select configuration step **406** may include determining whether a change in battery configuration is appropriate. For example, the previous/current battery configuration may be checked in light of a change in device operation, and if the configuration is appropriate for the change of device operation which has or is occurring, then the previous/current battery configuration may be left in place. Otherwise, a different configuration is selected.

Those skilled in the art will understand that reference to “ground” or a “ground node” indicates a reference node for the system and does not imply or require an actual connection to an earth ground or other external environment reference.

Those skilled in the art will recognize that the present invention may be manifested in a variety of forms other than the specific embodiments described and contemplated herein. Accordingly, departures in form and detail may be made without departing from the scope and spirit of the present invention as described in the appended claims.

What is claimed is:

1. An implantable medical device (IMD) comprising:

a housing configured for implantation in the body of a patient;

operational circuitry having low power monitoring sub-circuitry elements and high power stimulus generating sub-circuitry elements;

a power supply circuit coupled to the operational circuitry, the power supply circuit including at least first and second batteries and a plurality of switches, the power supply circuit configured to allow selective opening and closing of the switches such that the following output configurations are available:

a first configuration in which the first and second batteries are coupled in series to provide a low power output from only the first battery and a high power output from the first and second batteries in series; and

a second configuration in which the two batteries are isolated from one another to provide a low power output from only the first battery and a high power output from only the second battery;

wherein the operational circuitry is configured to perform the following method:

during a first time period, selecting the second configuration;

identifying one of the first or second batteries as having reduced output capacity; and

selecting the first configuration.

2. The IMD of claim 1, wherein the power supply circuit is further configured such that a third configuration is available, wherein in the third configuration, the first and second batteries are coupled in parallel to one another to provide an output from both batteries.

3. The IMD of claim 1, wherein the power supply circuit comprises a third battery and the first configuration provides the high power output from the first, second and third batteries in series.

4. The IMD of claim 3, wherein the power supply circuit comprises switches configured to omit one of the first, second or third batteries from use in supplying power.

5. The IMD of claim 1, wherein the power supply circuit comprises a third battery and the second configuration uses



## 11

the first battery alone to provide the low power output, and the second and third batteries in series to provide the high power output.

6. The IMD of claim 5, wherein the power supply circuit comprises switches configured to omit one of the first, second or third batteries from use in supplying power. 5

7. The IMD of claim 1, wherein the power supply circuit comprises switches configured to omit one of the first or second batteries from use in supplying power.

8. The IMD of claim 1, wherein the operational circuitry is configured to perform the following steps: 10

test at least one of the batteries to determine a status of the at least one battery;

select a configuration for the power supply circuit in light of the battery status; and 15

effect the configuration in the power supply circuit.

9. An implantable medical device (IMD) comprising a housing containing operational circuitry configured to operate the IMD, the operational circuitry comprising: 20

control circuitry for controlling operation of the IMD, the control circuitry operating using a low power circuit for power supply;

stimulus circuitry for providing an output stimulus to a patient during operation of the IMD, the stimulus circuitry operating, at least in part, by the use of a high power circuit for power supply; and

a battery system comprising at least a first battery, a second battery, and a plurality of switches coupling the first and second battery to a low power output and a high power output, the low power output coupled to the low power circuit for power supply and the high power output being coupled to the high power circuit for power supply, wherein the battery system and switches are coupled to the control circuitry such that the control circuitry can operate the switches in at least the following configurations: 25

## 12

(a) a configuration in which the low power circuit receives power from only the first battery and the high power circuit receives power from the first battery connected in series with the second battery; and

(b) a configuration in which the low power circuit and the high power circuit each receive power from the first battery and second battery connected in parallel such that the low power circuit and the high power circuit each receive similar voltage;

further wherein:

the battery system further comprises at least a third battery, and the plurality of switches also couples the third battery with the first and second batteries such that the control circuitry can also operate the switches in (c) a configuration in which at least one of the first, second and third batteries is excluded from use;

the control circuitry includes means for testing battery status of one or more of the batteries; and

the control circuitry is configured to perform a power configuration method comprising the following steps: testing battery status of at least one of the batteries; selecting a battery configuration; and effecting the selected battery configuration.

10. The IMD of claim 9, wherein the control circuitry is further configured to perform the power configuration method at intervals. 25

11. The IMD of claim 9, wherein the control circuitry is further configured to perform the power configuration in response to a change in device operation.

12. The IMD of claim 11, wherein the change in device operation is a determination by the control circuitry that cardiac stimulus is indicated. 30

13. The IMD of claim 11, wherein the change in device operation is a time-out occurring during preparation of the stimulus circuitry to provide a stimulus. 35

\* \* \* \* \*