

US008491302B2

(12) **United States Patent**
Arni

(10) **Patent No.:** **US 8,491,302 B2**
(45) **Date of Patent:** **Jul. 23, 2013**

(54) **DENTAL IMPLANT**

(56) **References Cited**

(76) Inventor: **Uri Arni**, Beer Yaacov (IL)

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 575 days.

5,427,527	A	6/1995	Niznick et al.
5,816,812	A	10/1998	Kownacki et al.
5,964,768	A	10/1999	Huebner
6,030,162	A	2/2000	Huebner
6,547,564	B1	4/2003	Hansson
2004/0006346	A1	1/2004	Holmen et al.
2004/0063071	A1	4/2004	Schroering
2004/0219488	A1	11/2004	Choi et al.
2005/0131413	A1*	6/2005	O'Driscoll et al. 606/73
2005/0276676	A1	12/2005	Mardinger et al.
2007/0233122	A1*	10/2007	Denis et al. 606/73

(21) Appl. No.: **12/293,787**

(22) PCT Filed: **Mar. 21, 2007**

(86) PCT No.: **PCT/IL2007/000369**

§ 371 (c)(1),
(2), (4) Date: **Aug. 6, 2010**

FOREIGN PATENT DOCUMENTS

(87) PCT Pub. No.: **WO2007/107995**

PCT Pub. Date: **Sep. 27, 2007**

EP	0 412 845	2/1991
EP	0 705 572	4/1996
EP	0 705 572 A2	4/1996

OTHER PUBLICATIONS

Office Action for Israeli Patent Application No. 194200 mailed on Oct. 9, 2011; 3 pages.

(65) **Prior Publication Data**

US 2011/0045437 A1 Feb. 24, 2011

* cited by examiner

Primary Examiner — Yogesh Patel

(74) *Attorney, Agent, or Firm* — Shichrur & Co.

Related U.S. Application Data

(60) Provisional application No. 60/784,833, filed on Mar. 21, 2006.

(51) **Int. Cl.**
A61C 8/00 (2006.01)
A61C 13/225 (2006.01)


(52) **U.S. Cl.**
USPC **433/173**; 433/172



(58) **Field of Classification Search**
USPC 433/172–176, 201.1; 606/264–272,
606/275, 300–321; 411/412, 413, 307
See application file for complete search history.

(57) **ABSTRACT**

A dental implant with a coarsely threaded portion suitable for nesting within the cortical bone, and a finely threaded portion suitable for nesting within the cancellous bone. A primary thread with a constant pitch and a constant major diameter, runs along both the finely threaded portion and the coarsely threaded portion, and has a large thread height in the coarsely threaded portion, and a small thread height in the finely threaded portion. At least one secondary thread, having the constant pitch and the small thread height, runs along the finely threaded portion at an offset from the primary thread.

13 Claims, 6 Drawing Sheets

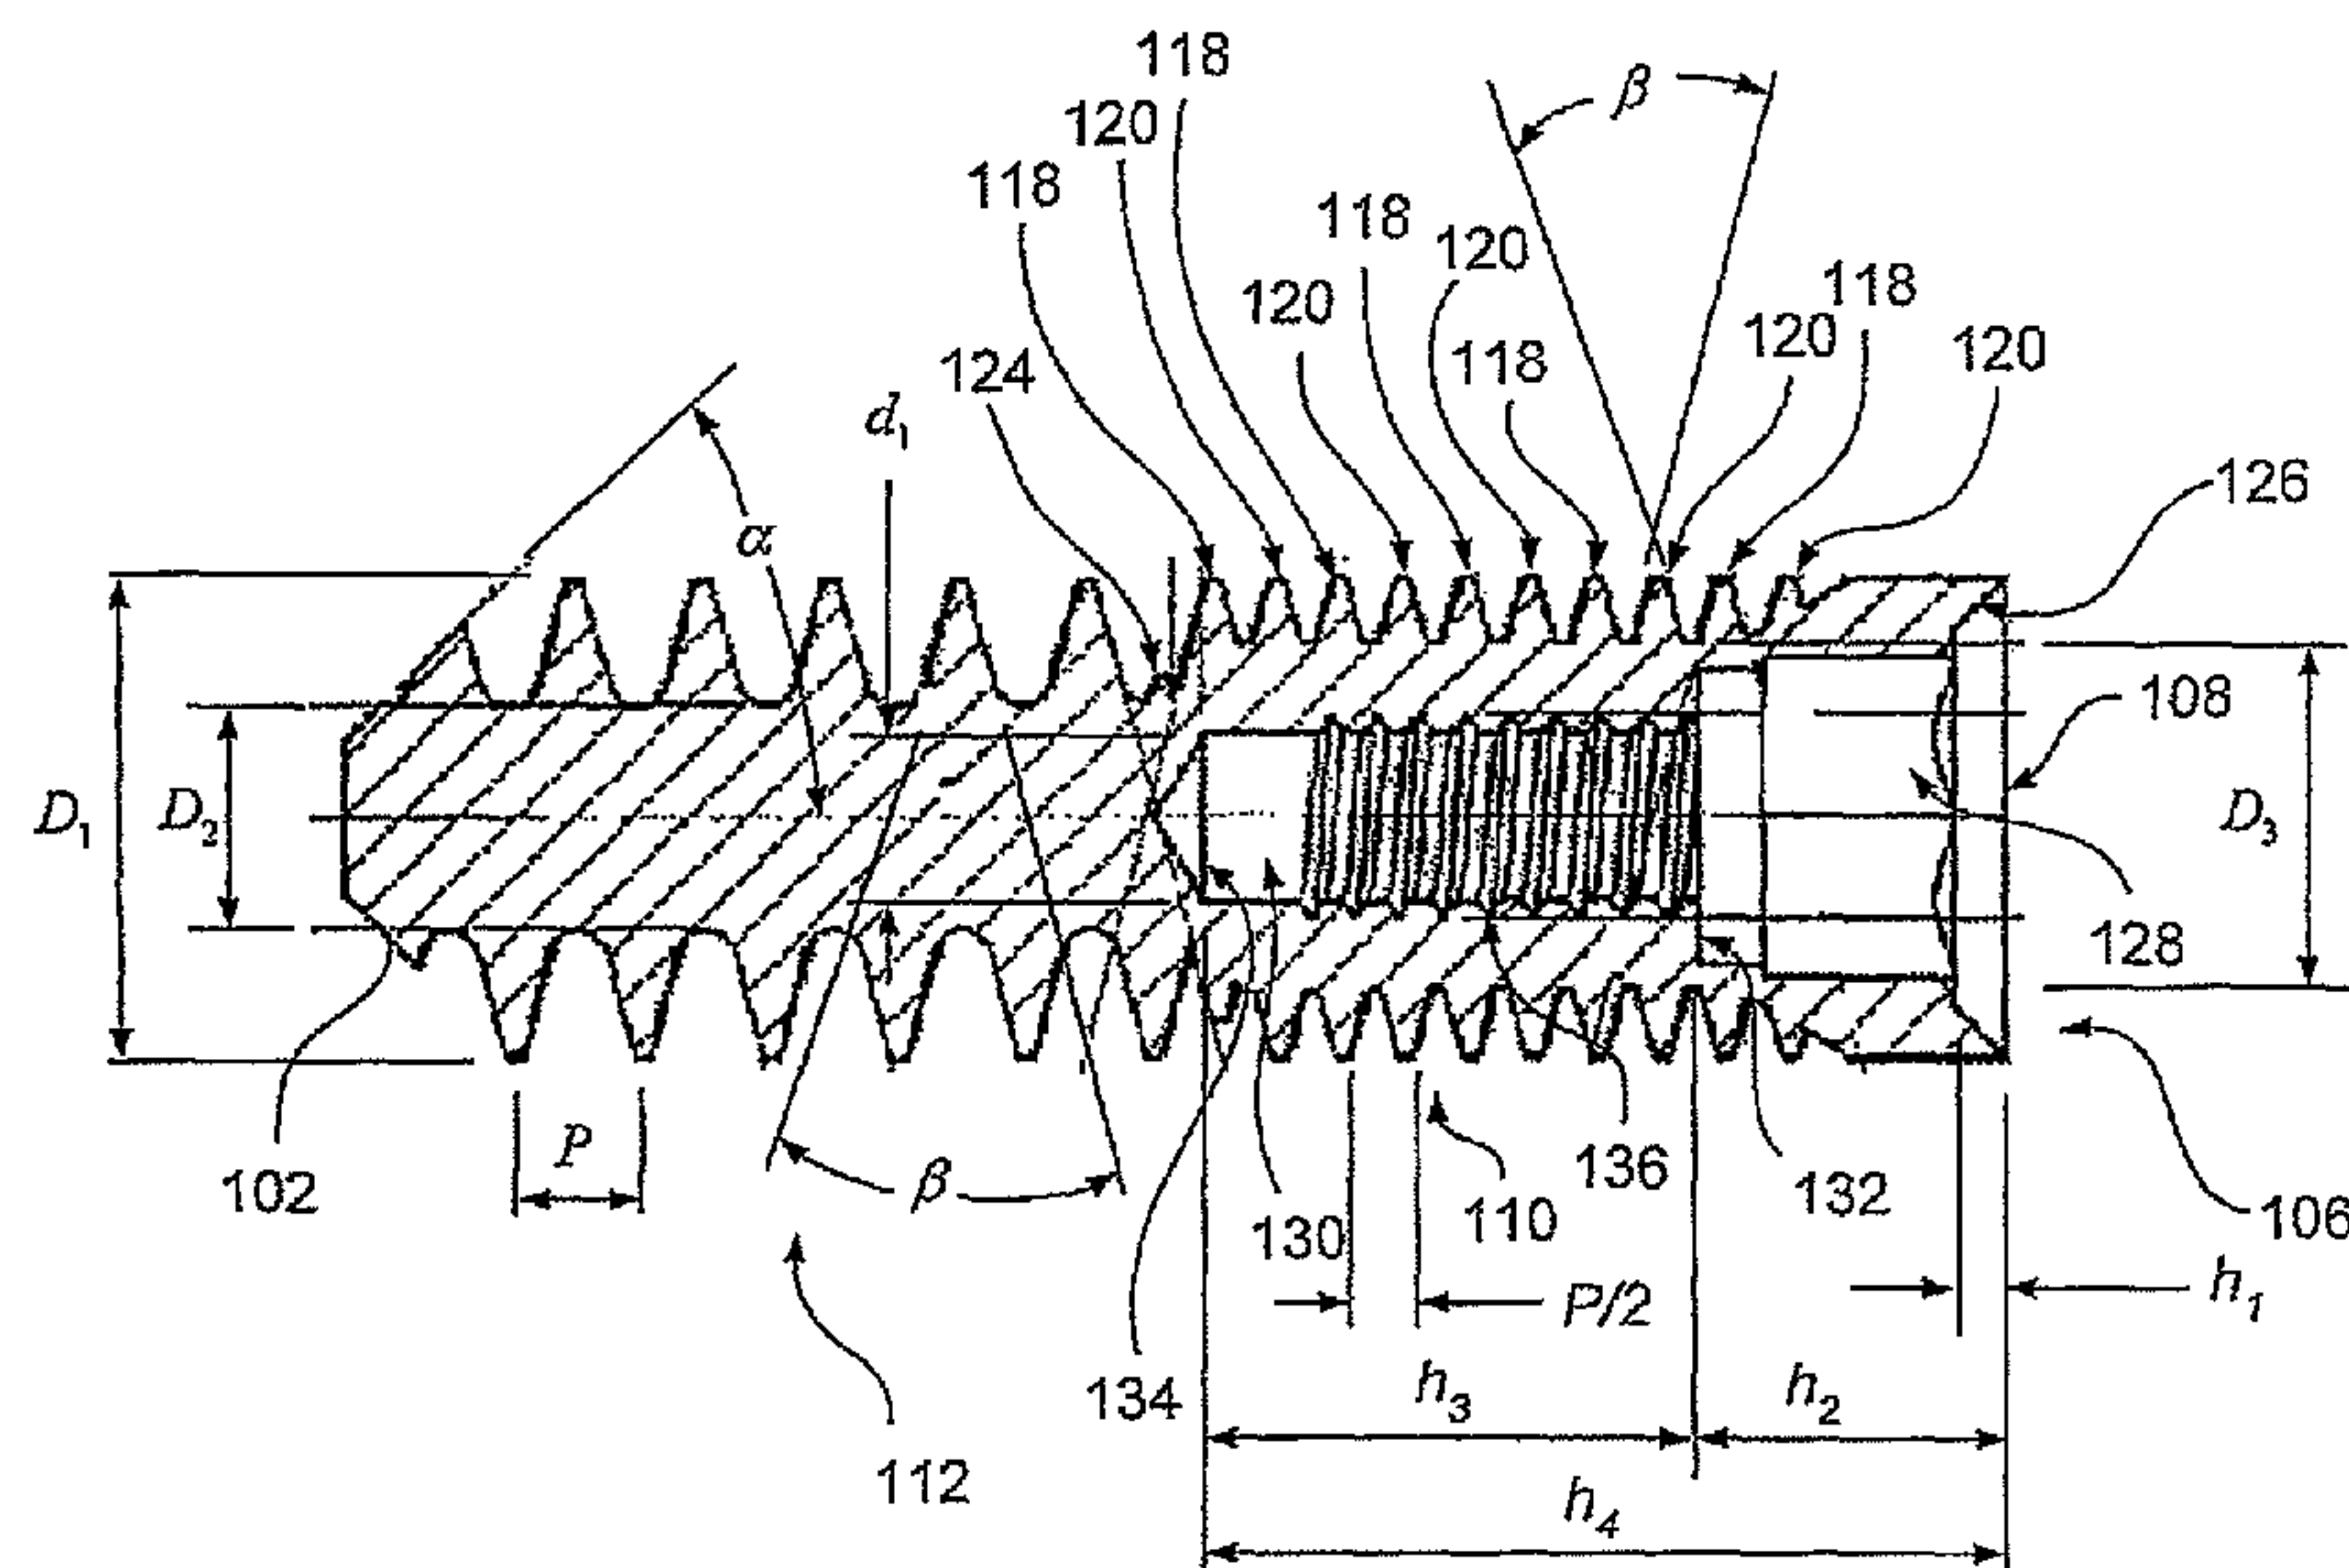

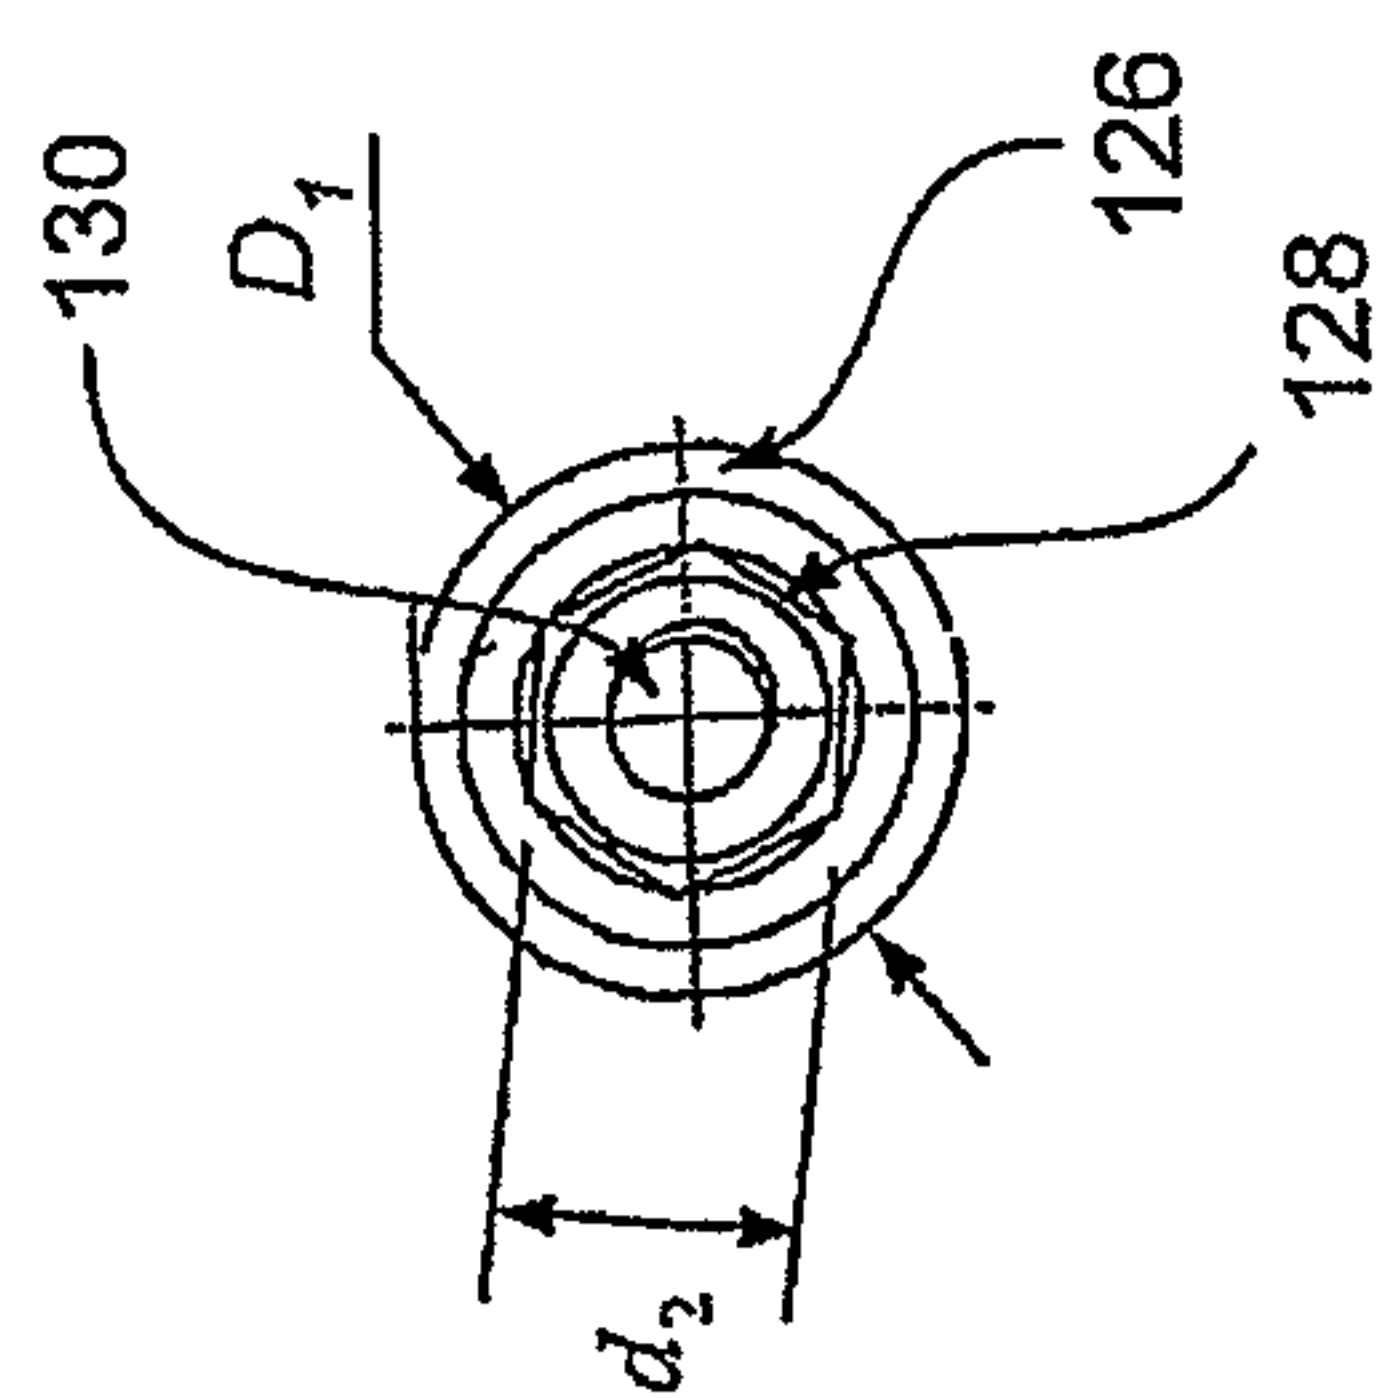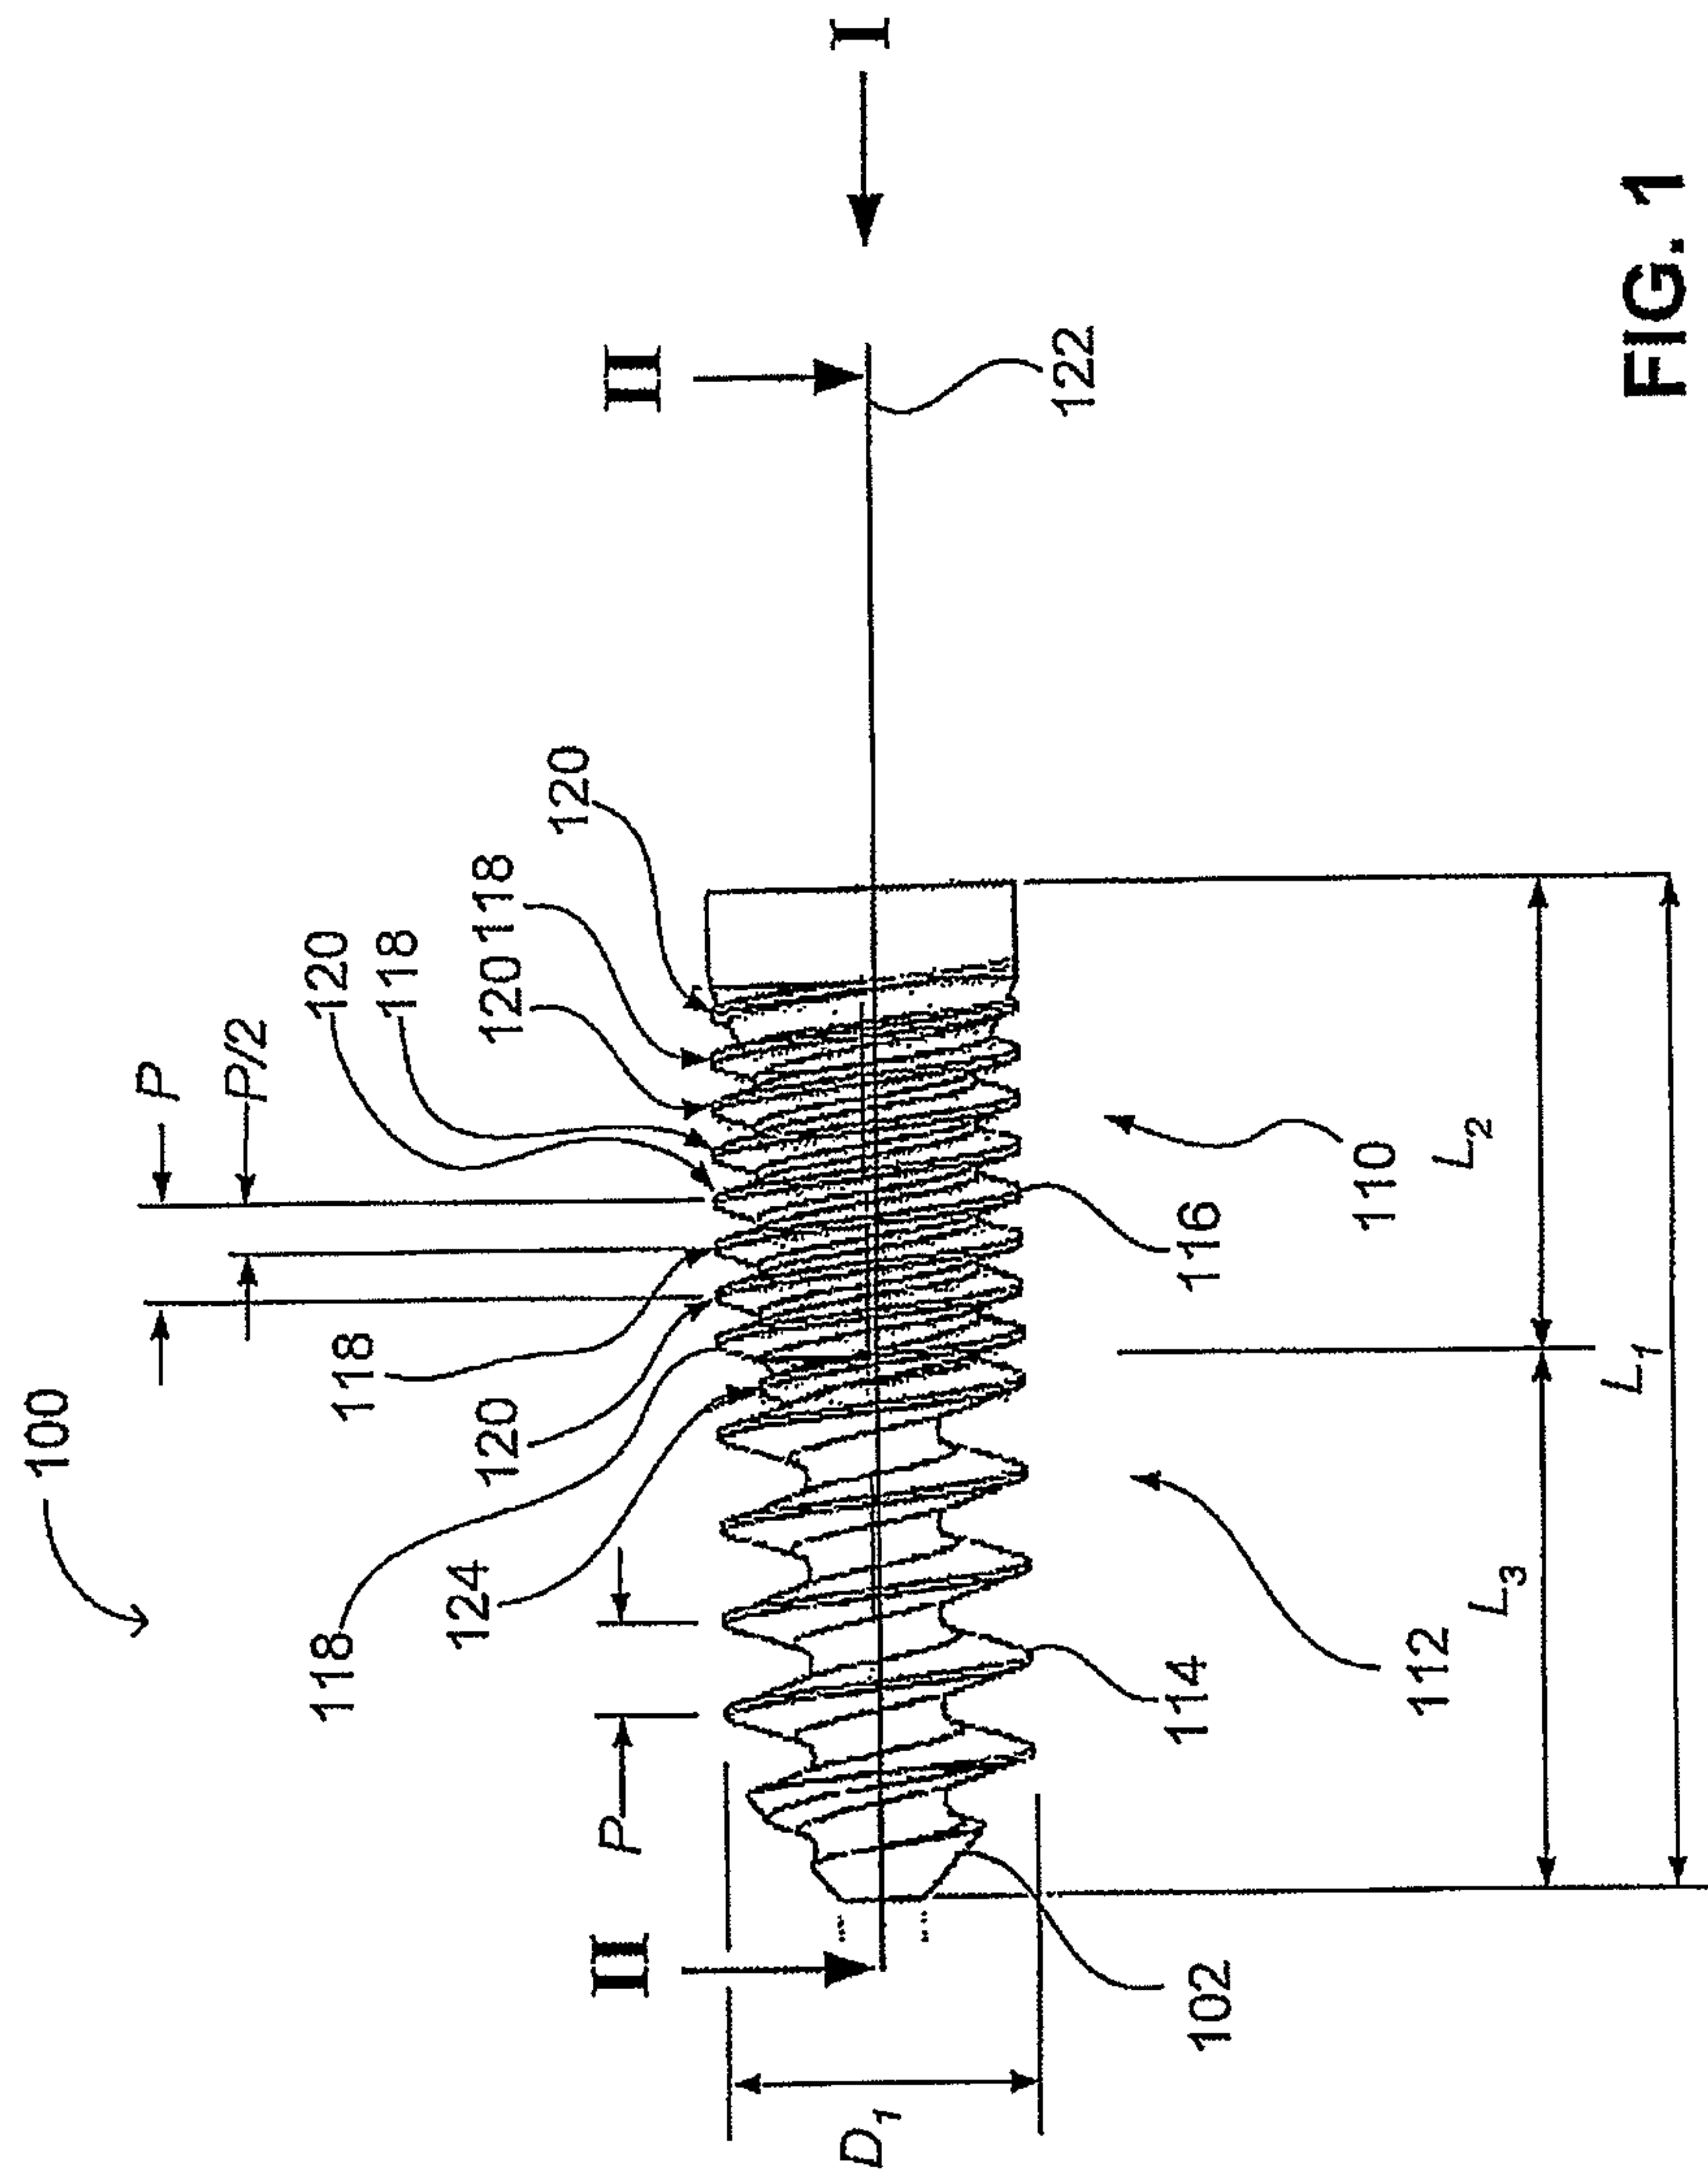

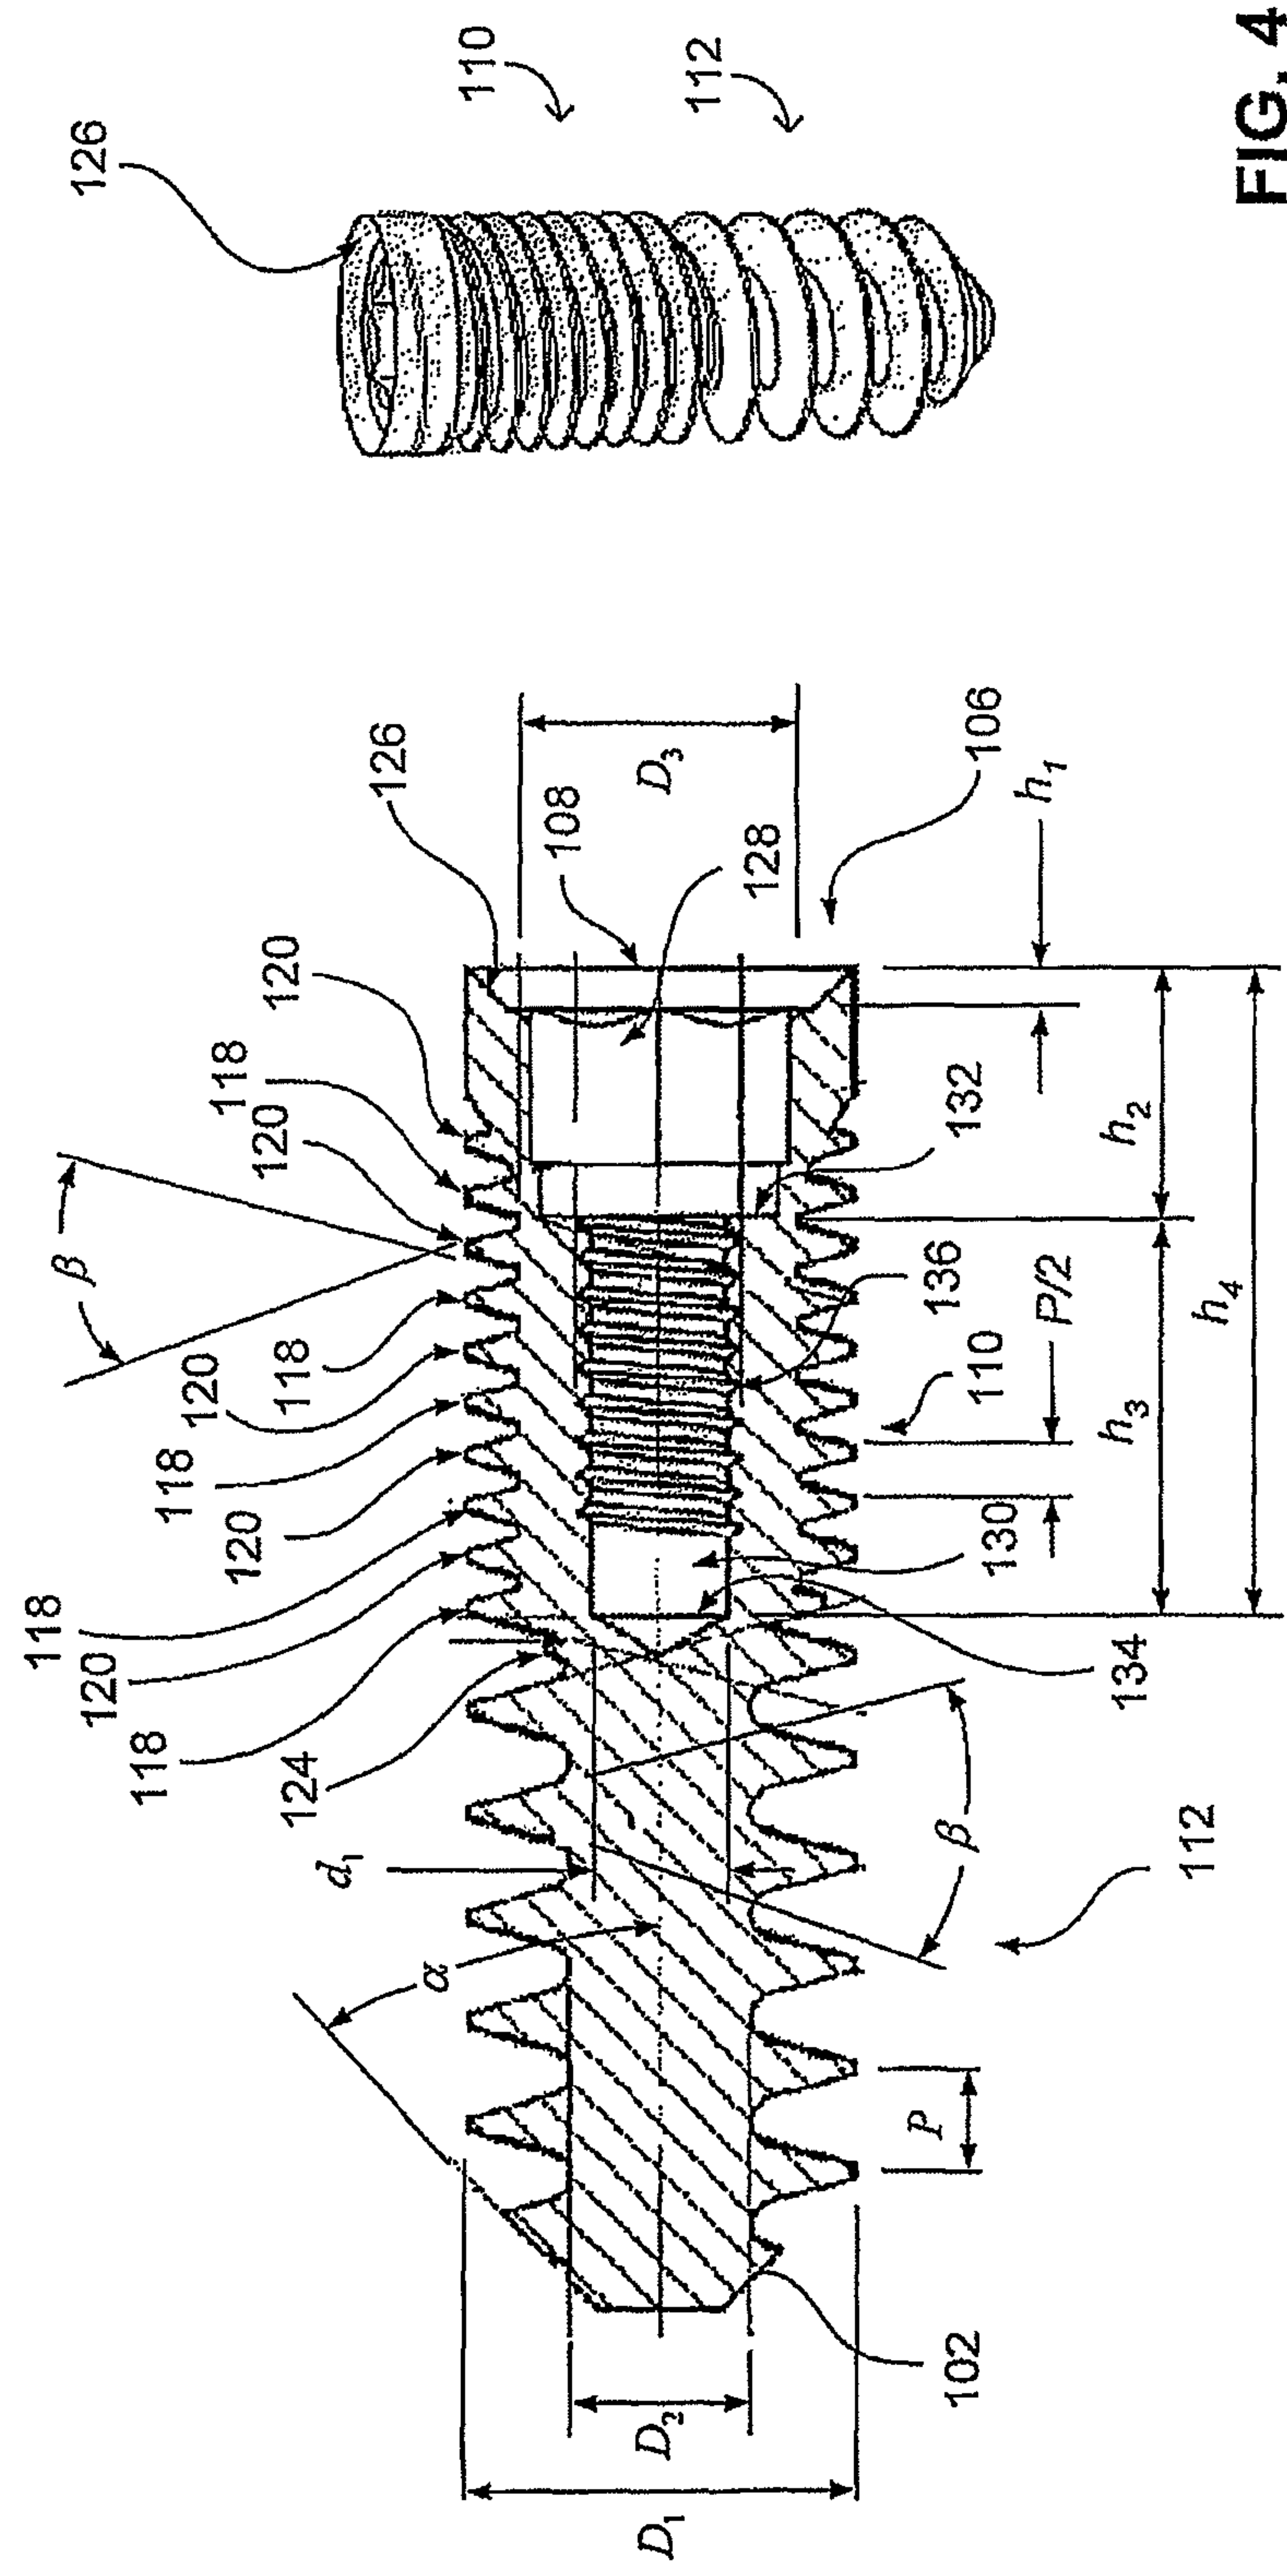
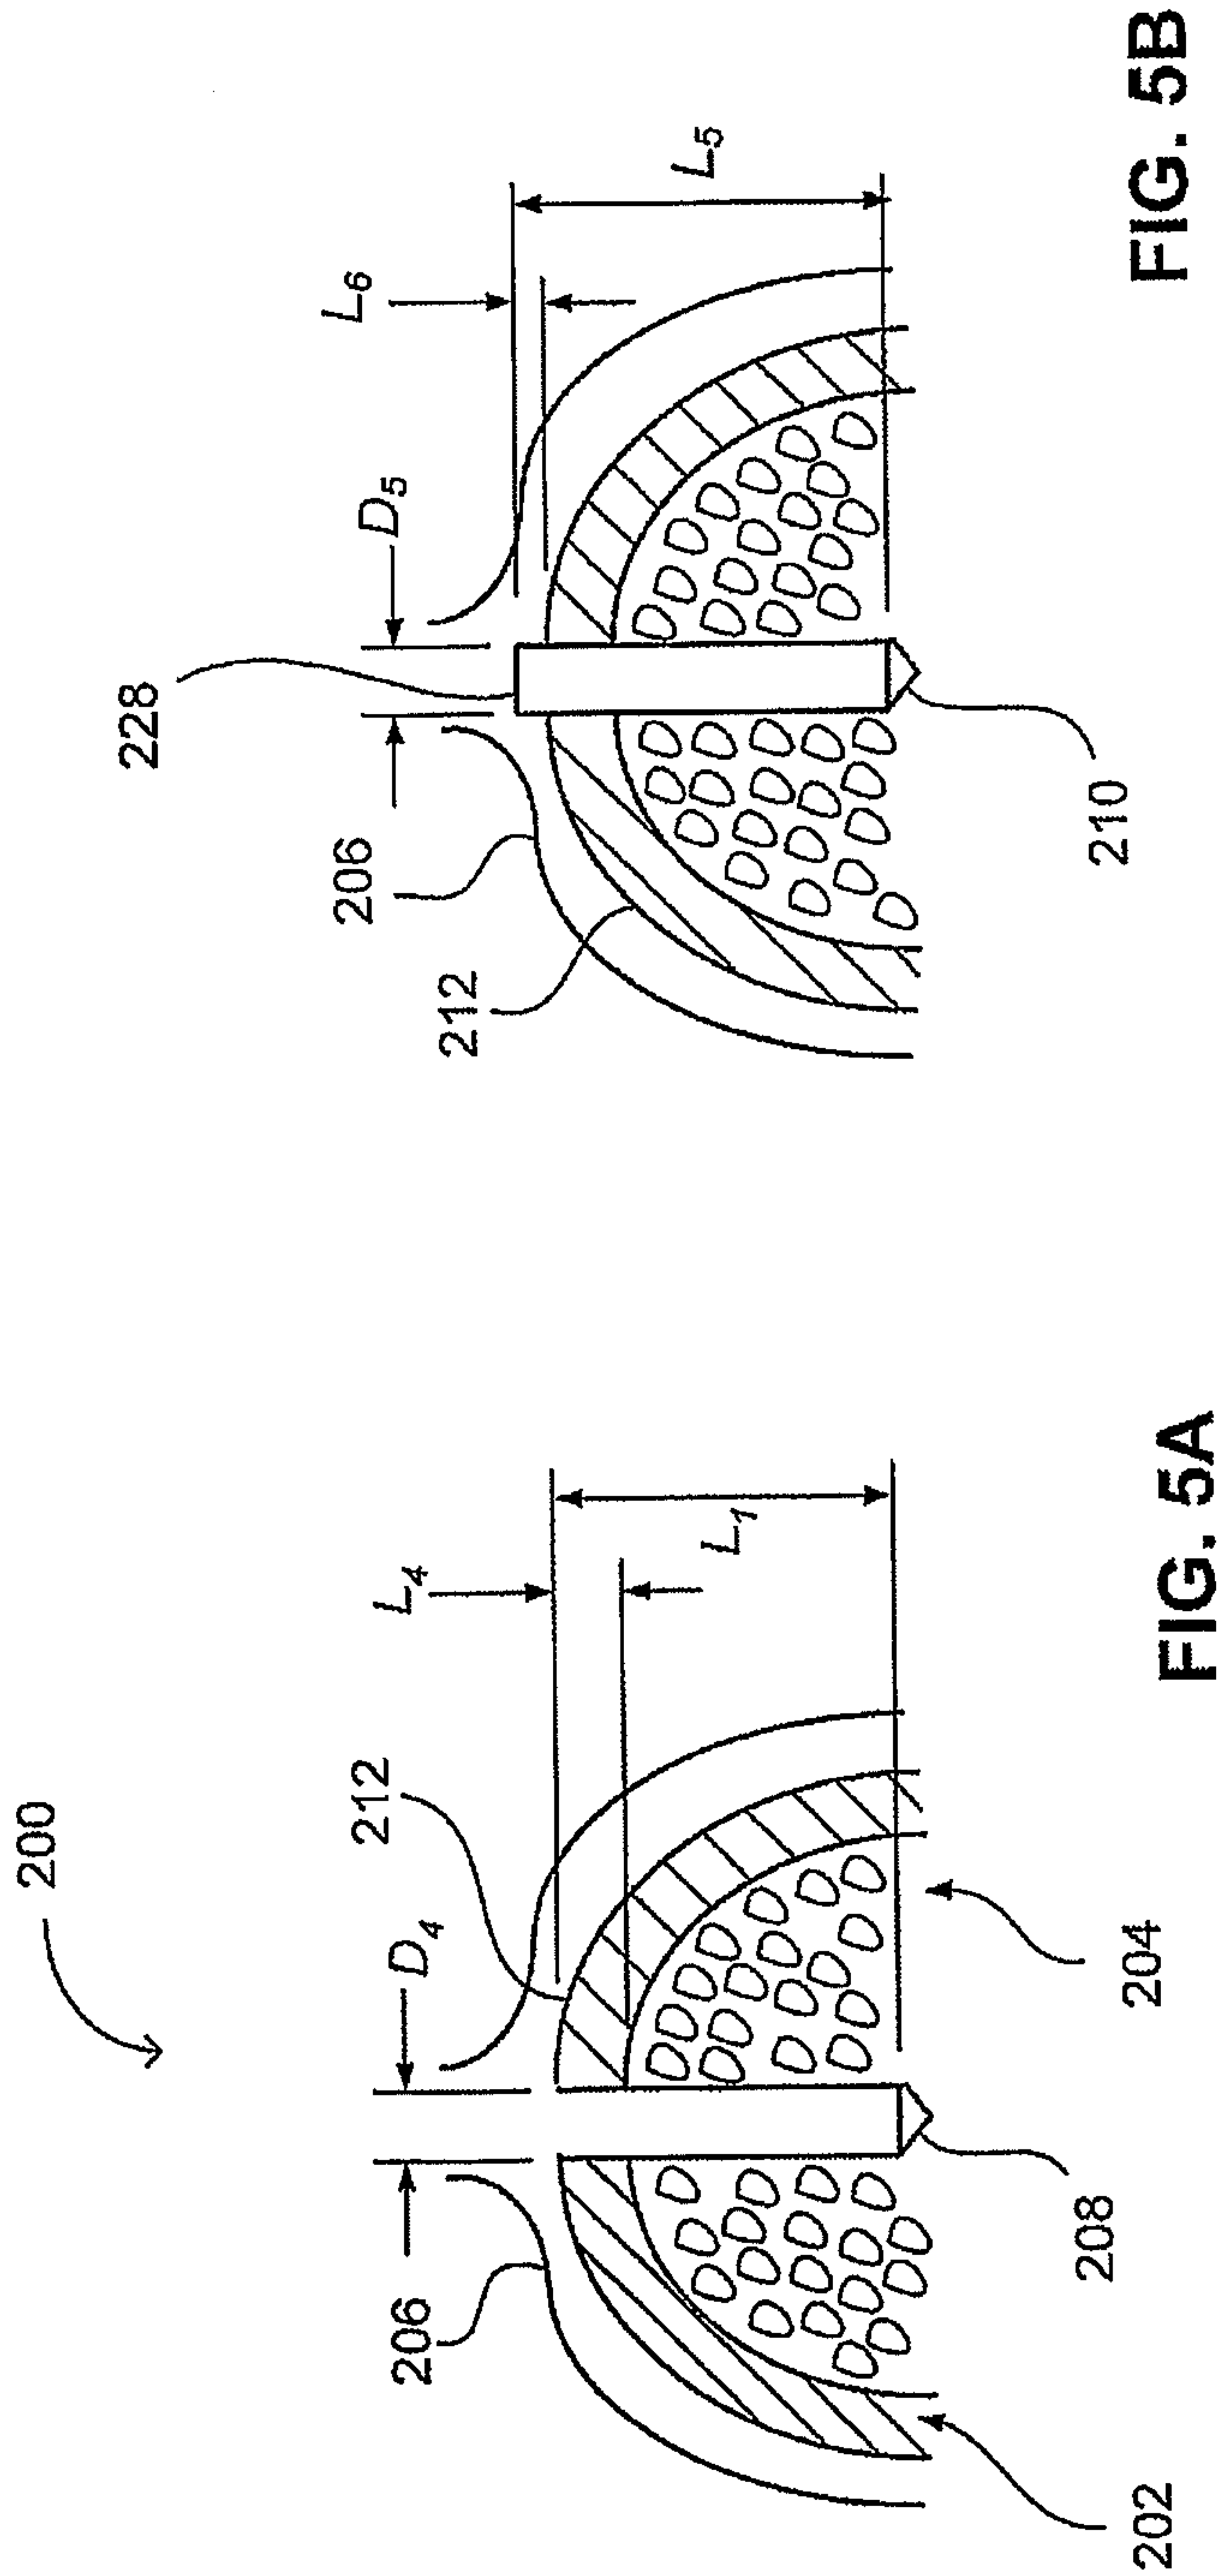


FIG. 3

FIG. 4



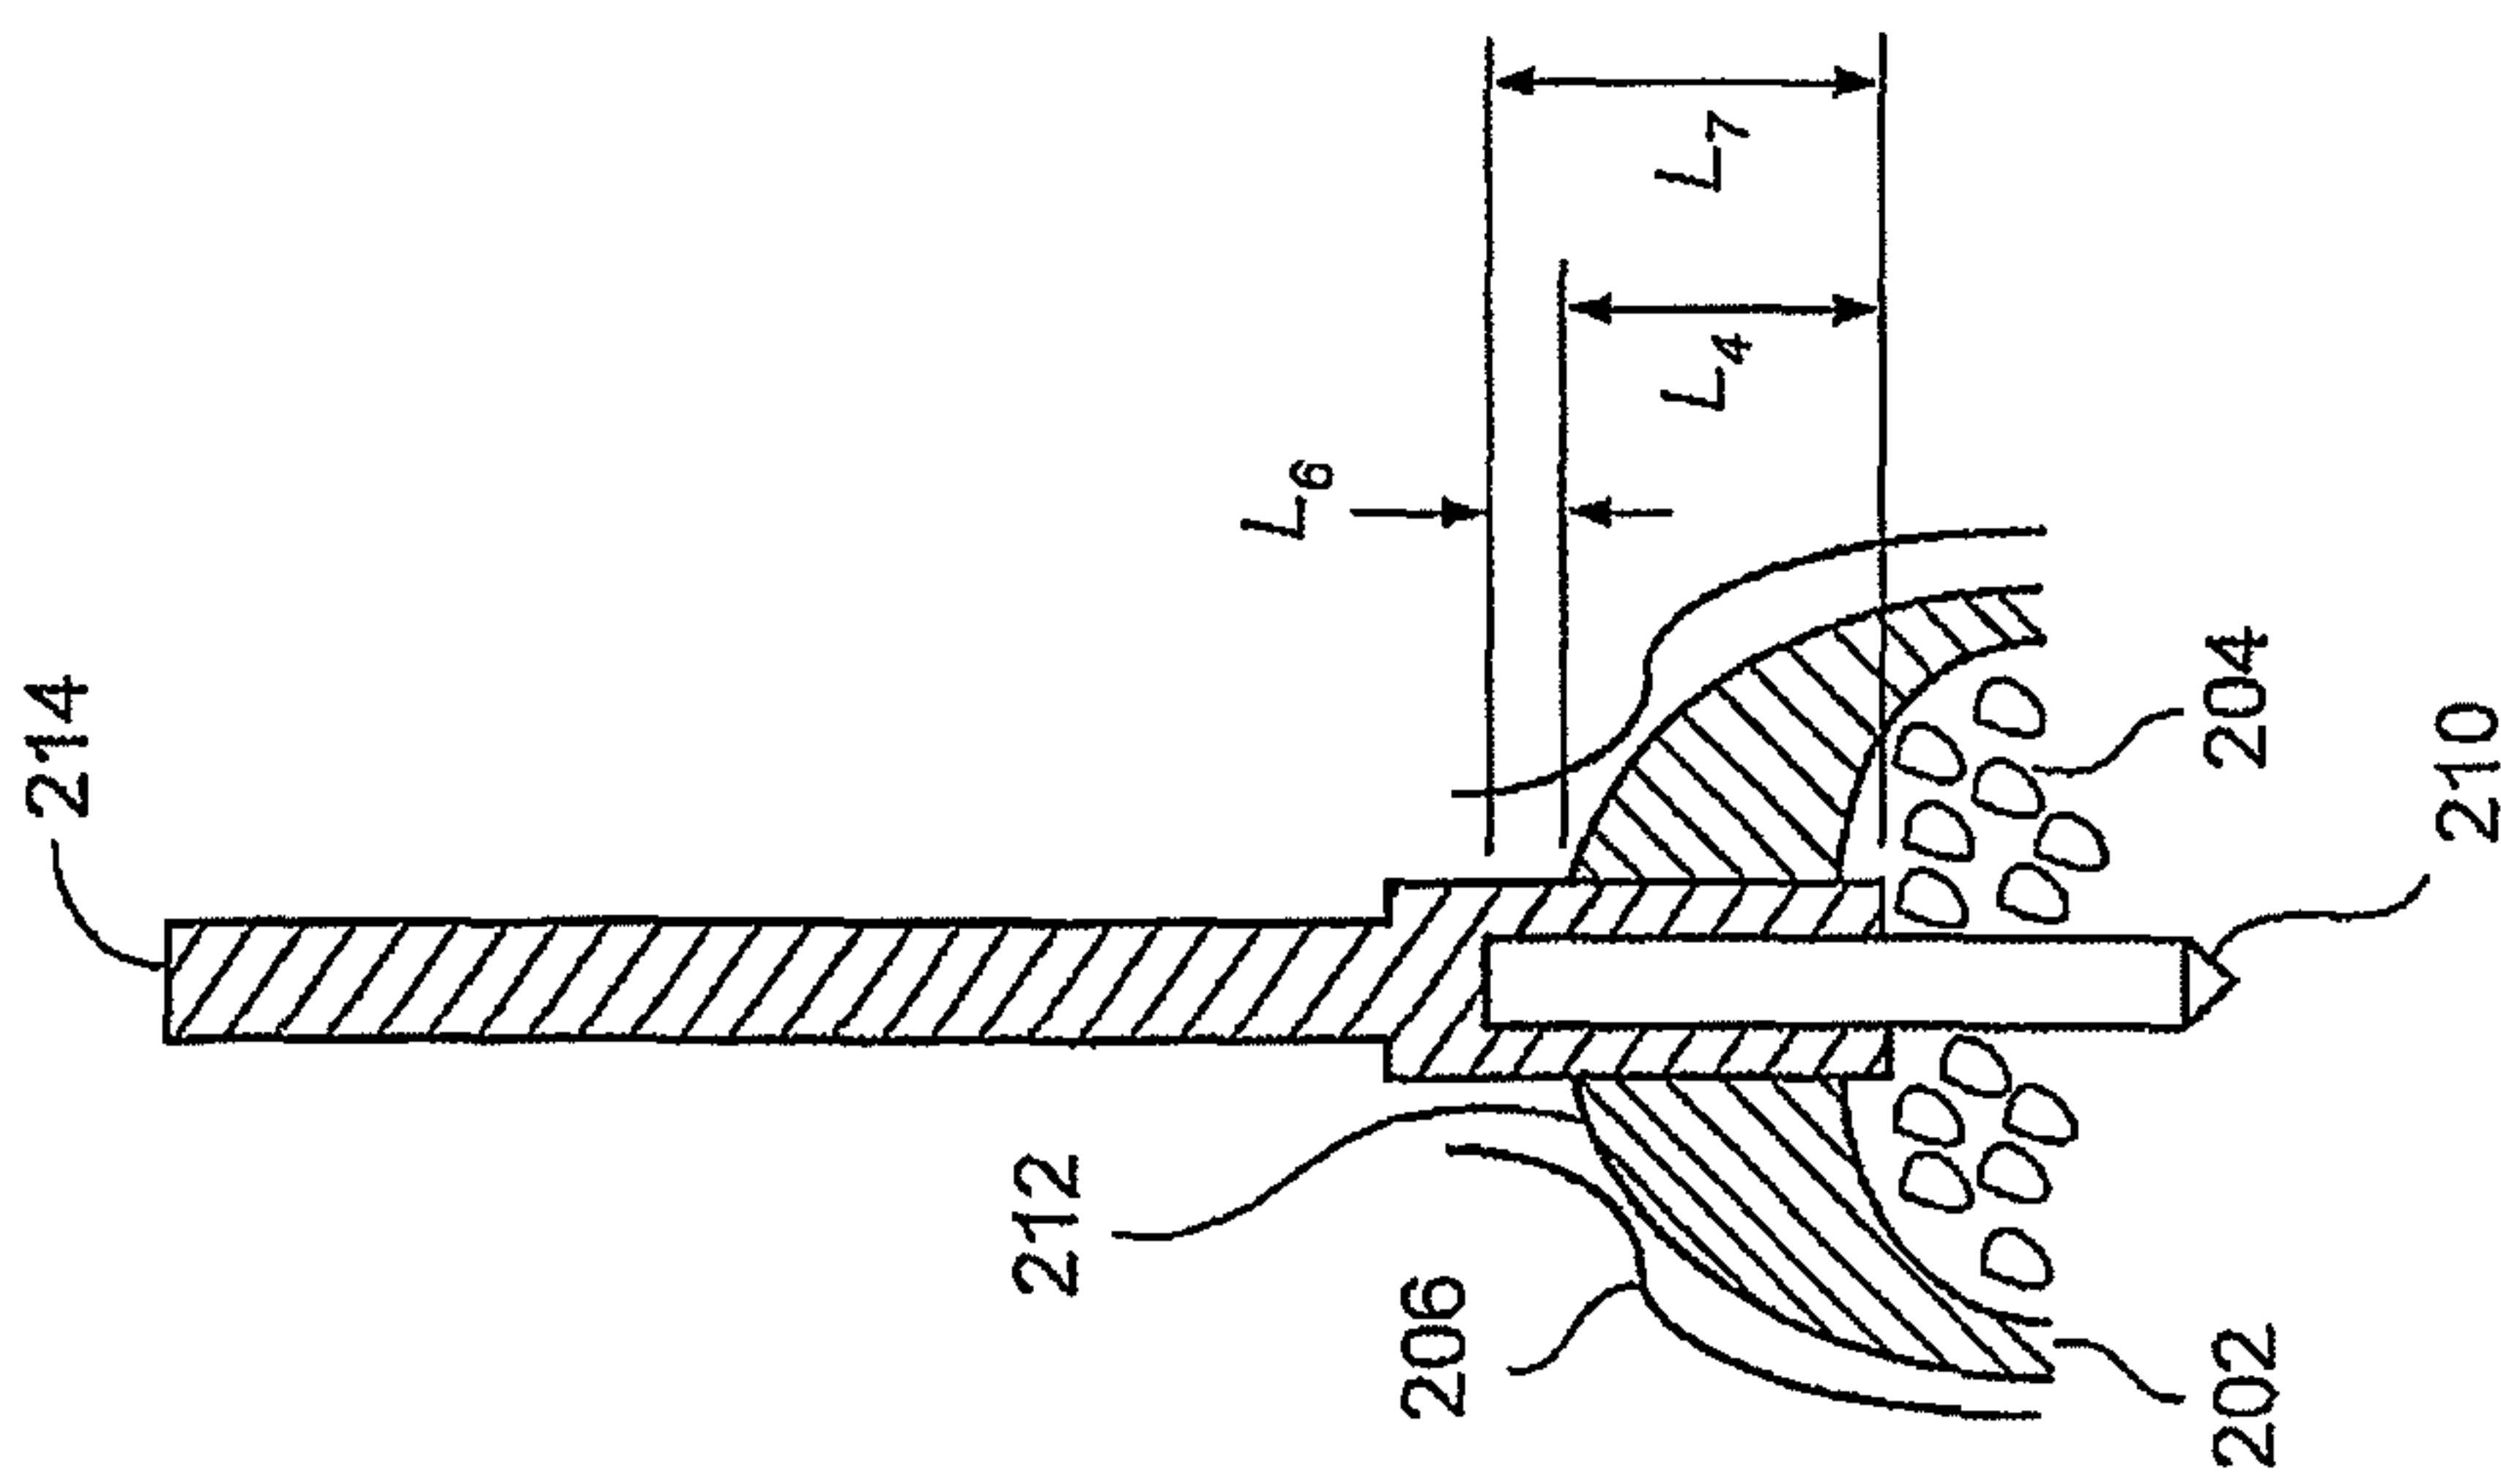


FIG. 5C

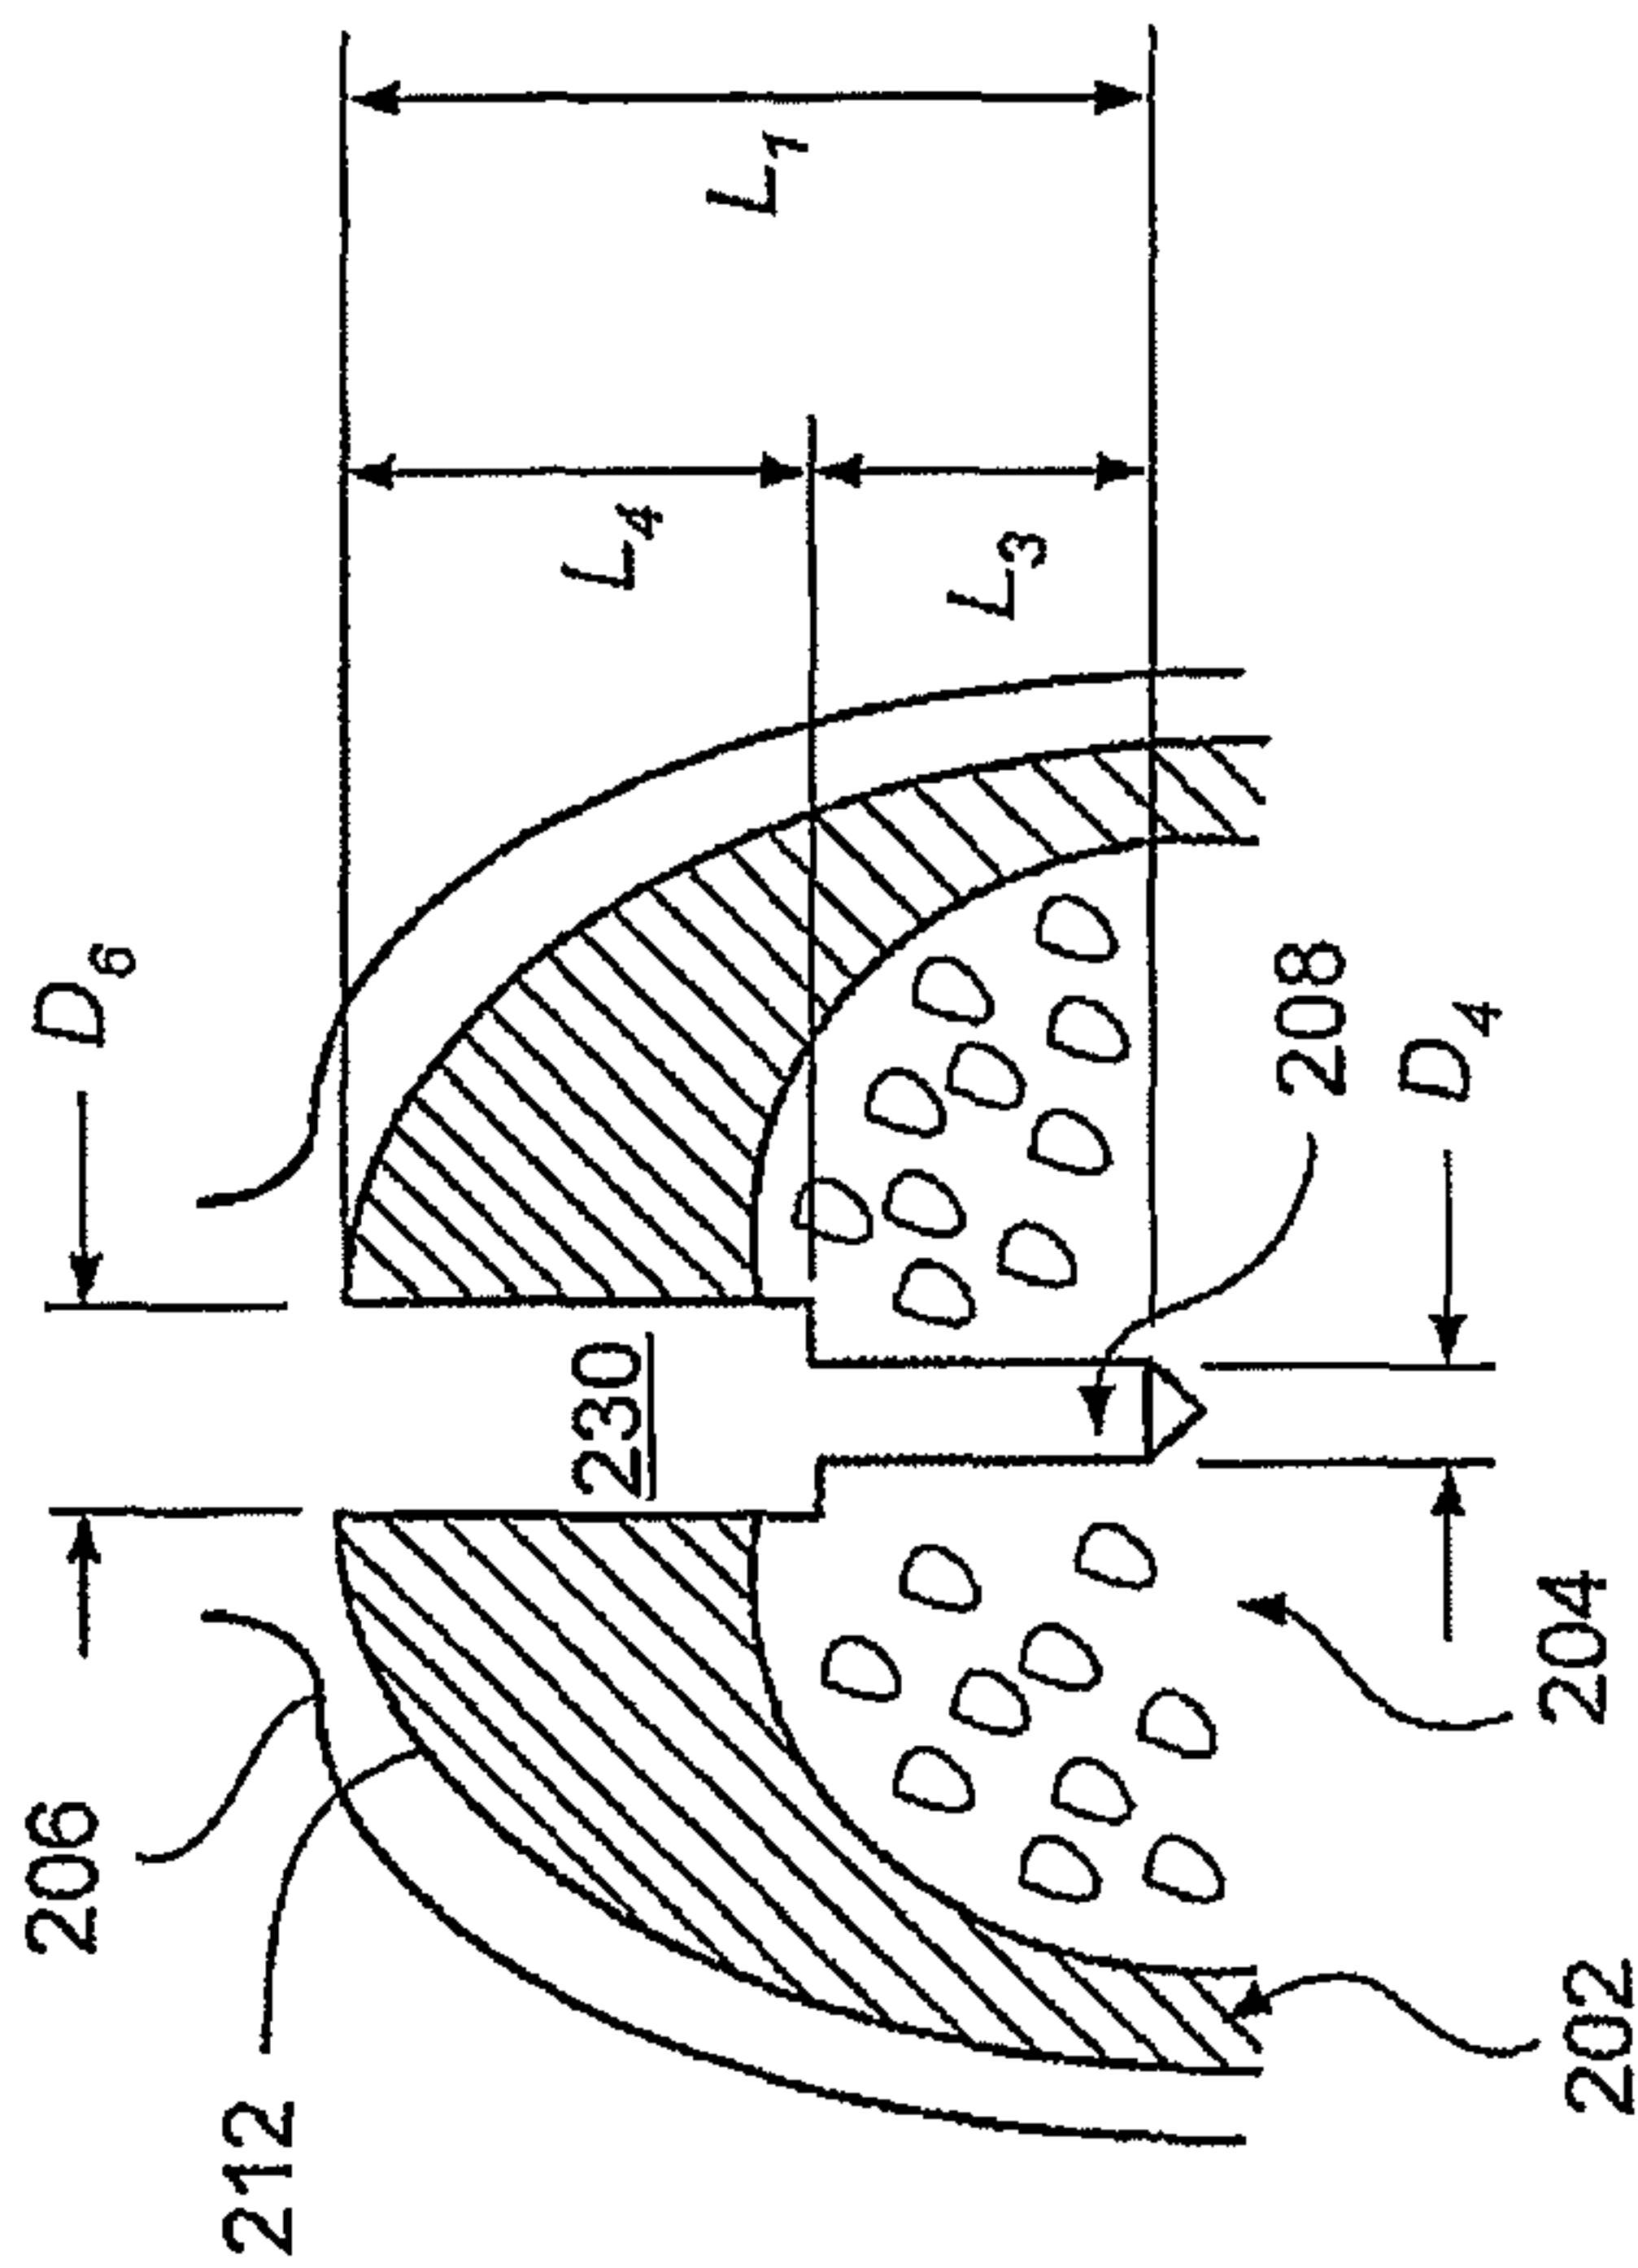


FIG. 5D

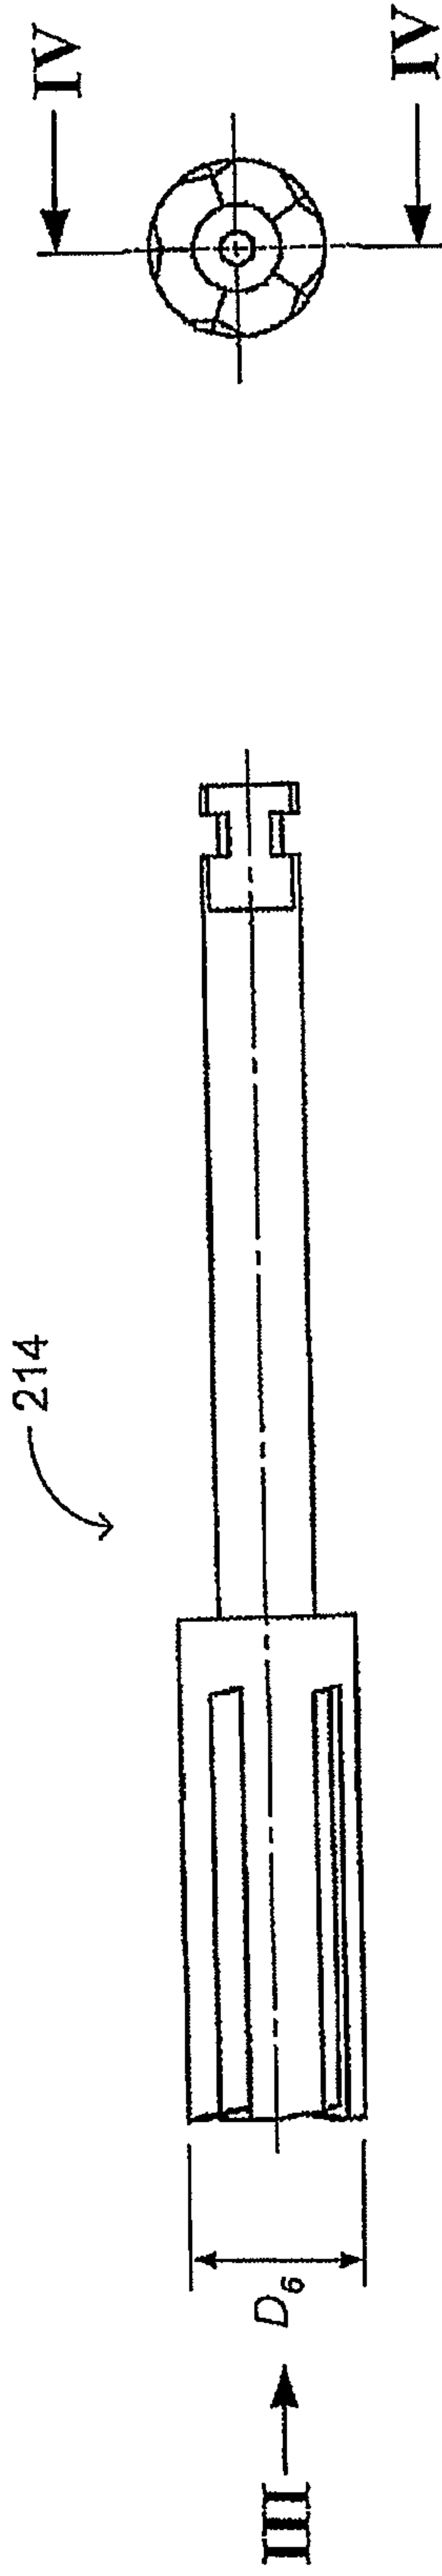


FIG. 6


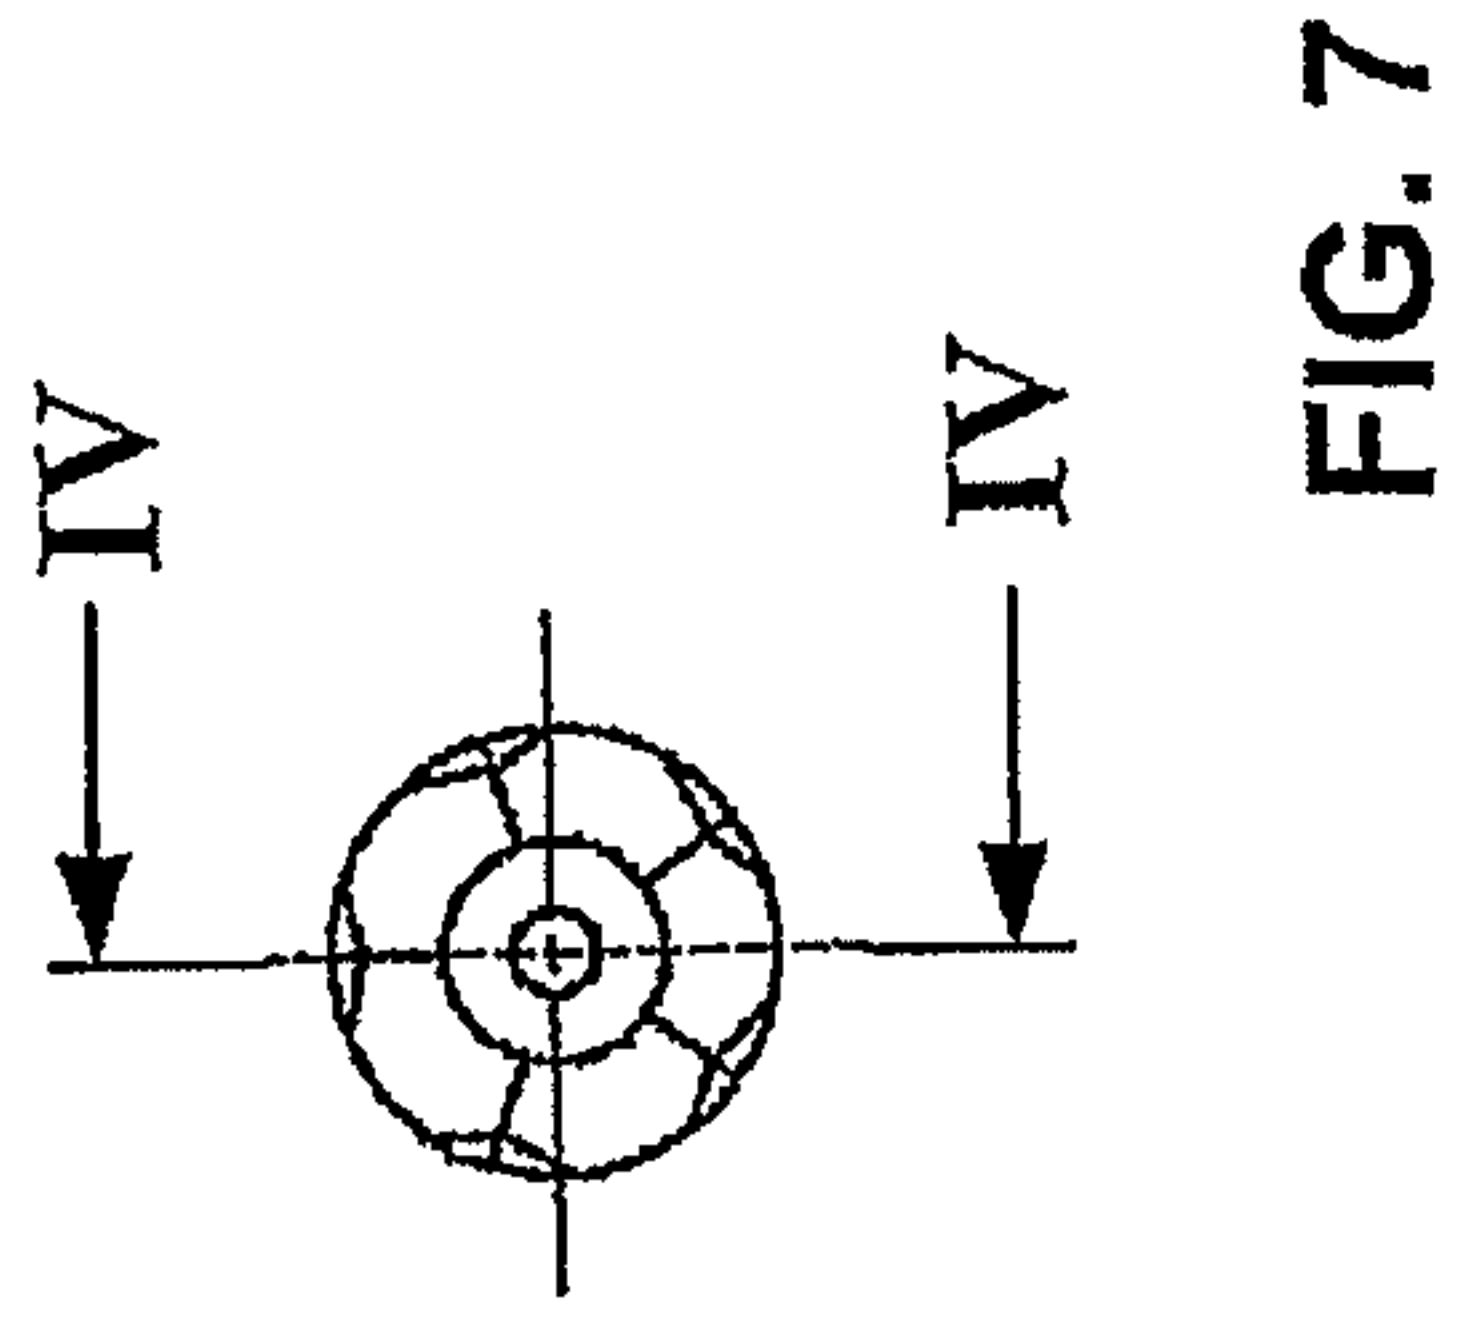


FIG. 7

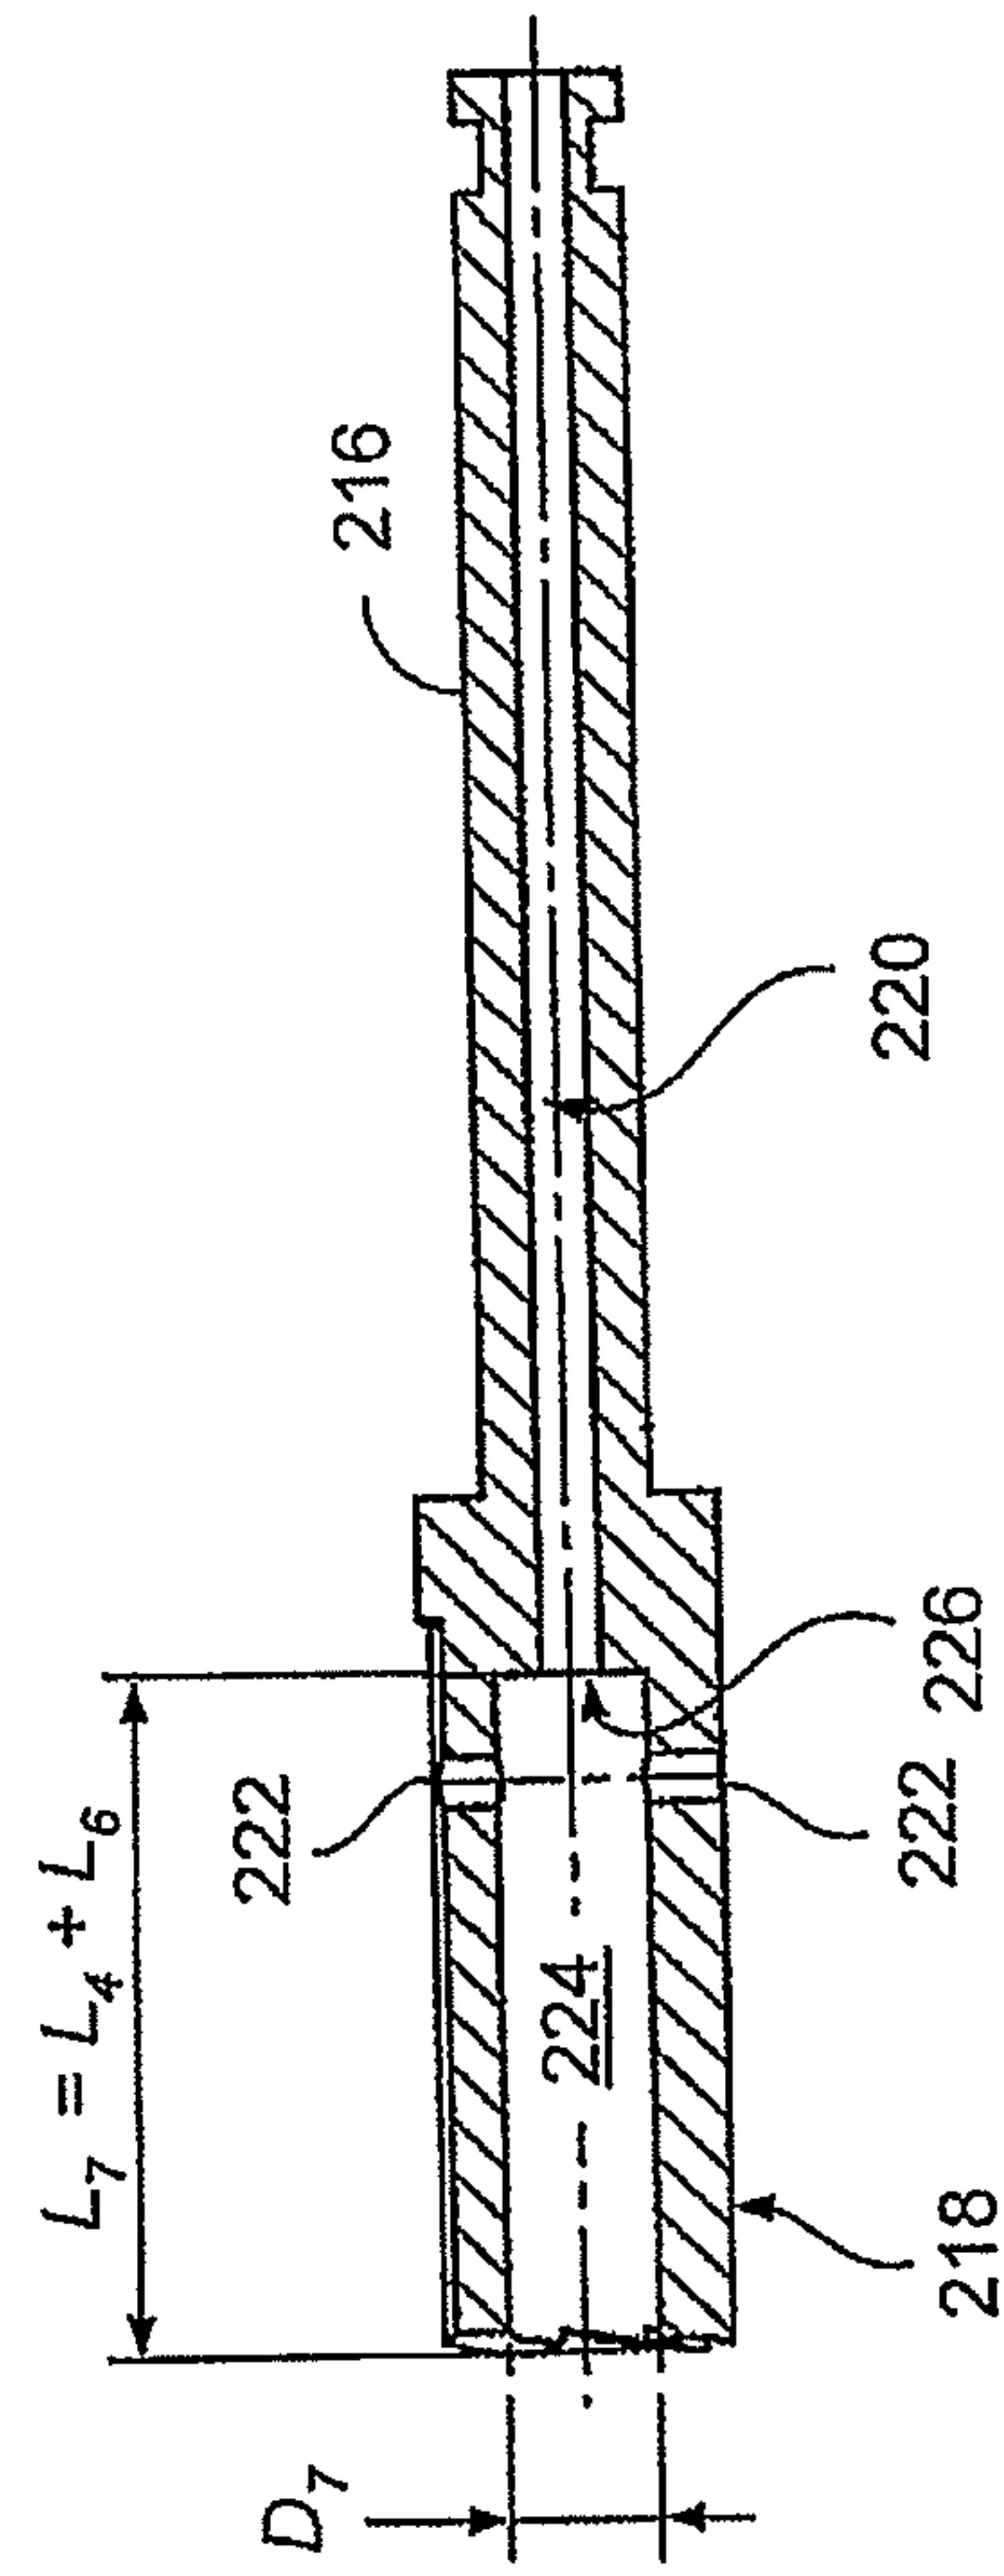

8
C
LL

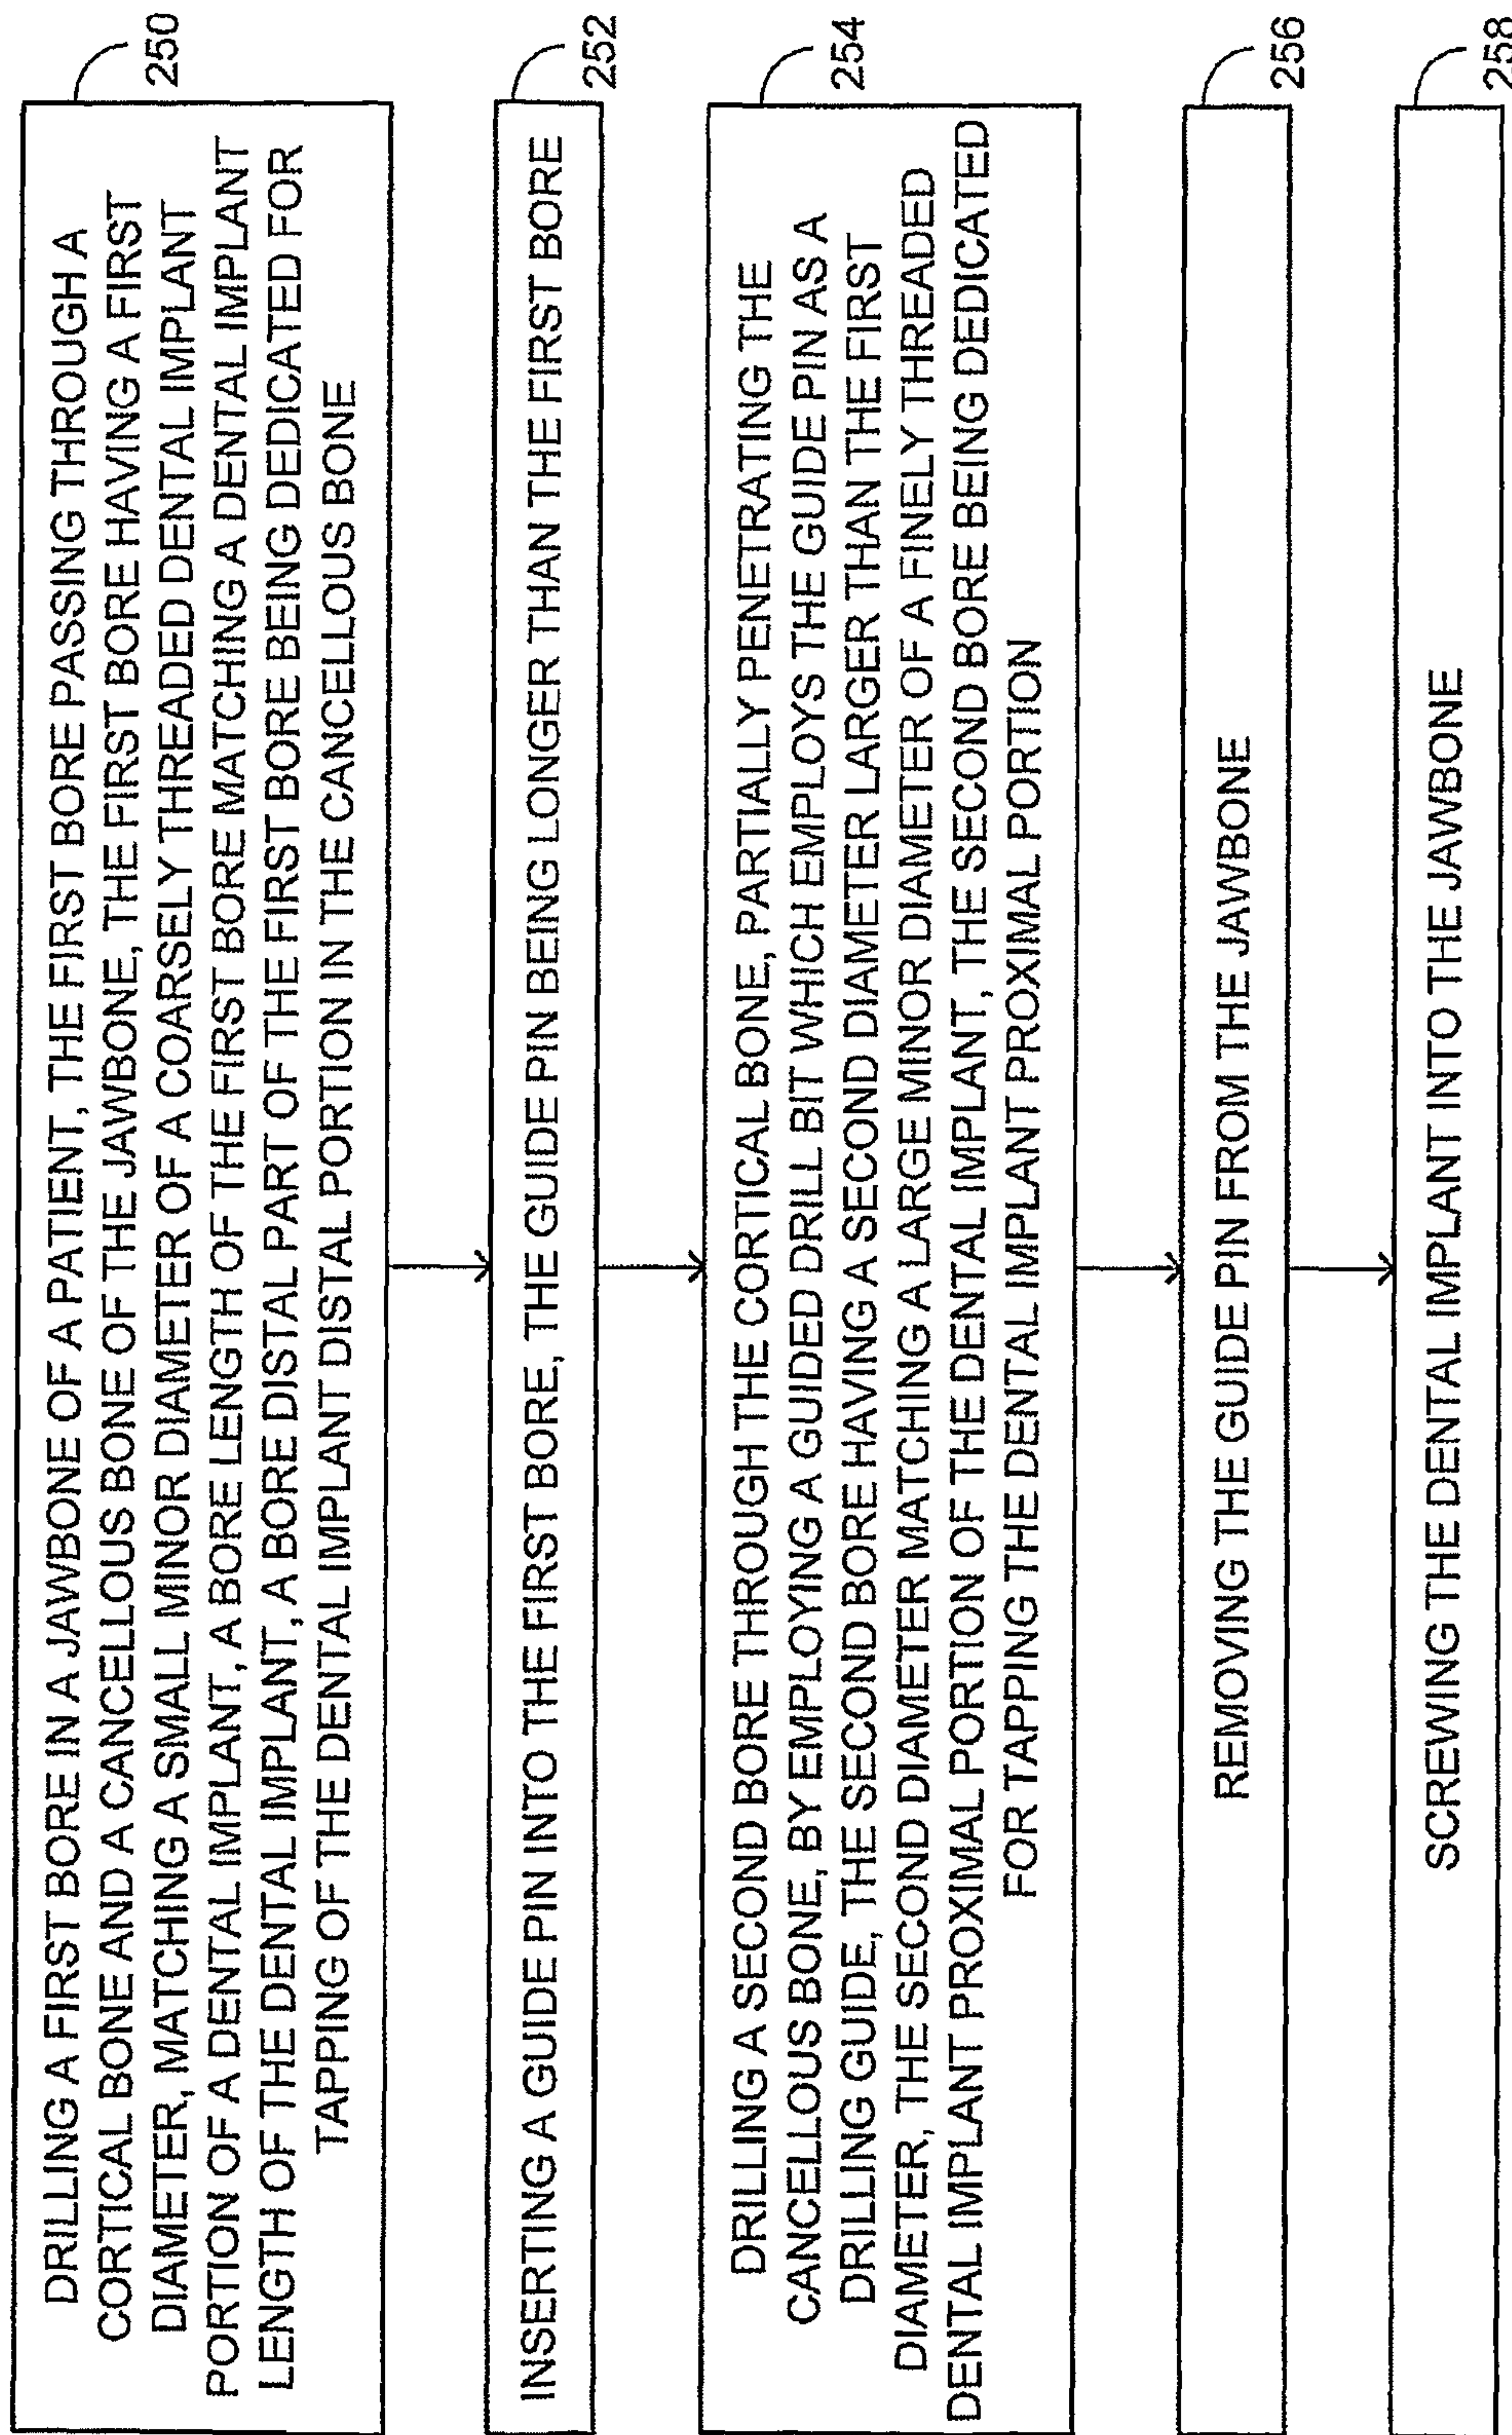


FIG. 9

DENTAL IMPLANT

This application is a National Stage Application of PCT/IL2007/000369, filed 21 Mar. 2007, which claims benefit of U.S. application Ser. No. 60/784,833, filed 21 Mar. 2006 and which applications are incorporated herein by reference. To the extent appropriate, a claim of priority is made to each of the above disclosed applications.

FIELD OF THE INVENTION

The disclosed technique relates to medical devices in general, and to methods and systems for performing a dental implant, in particular.

BACKGROUND OF THE INVENTION

A tooth can be implanted by inserting a dental implant into the jawbone (i.e., either the mandible or the maxilla), and by attaching a substitute or an artificial tooth to the dental implant. Generally, the dental implant is in form of an externally threaded screw, which is screwed into a pre-drilled bore of the jawbone, at an appropriate diameter. A major problem with dental implants is the dislodging of the dental implant, after a certain period of use, due to the forces which act on the dental implant during mastication.

Screw profiles and anchoring means directed to increase the bonding forces between the jawbone, and the dental implant, and to increase the life of the dental implant are known in the art. One such anchoring means utilizes grooves and holes in the body of the dental implant, to allow the osseous cells to grow into the grooves and the holes. Other anchoring means utilize screw threads of different pitches along the length of the anchoring means.

A major cause of dislodging of the anchoring means is insufficient bonding area. This problem is especially pronounced in the cancellous bone of the mandible and the maxilla, which is porous and therefore much weaker than the compact cortical bone. The cancellous bone is located beneath the cortical bone, and very often the anchoring forces which act between the dental implant and the cancellous bone are very small, thereby lending the bottom portion of the dental implant, which enters into the cancellous bone, literally useless.

U.S. Pat. No. 6,547,564 issued to Hansson, and entitled "Bone Implant Having Circumferentially Oriented Roughness", is directed to a self tapping endosseous screw-type dental implant. The dental implant has an apical end, an intermediate section, and a coronal end. The apical end is presented by a first conical section. The coronal end is presented by a second conical section. The intermediate section is of a constant diameter, and extends from the apical end to the coronal end. The outer surface of the dental implant is provided with a screw threading which is divided into a coronal section and an apical section. The coronal section is positioned on the intermediate section. The apical section bridges the intermediate section and the first conical section.

The screw thread in the coronal section is in form of microthreads, having a height which is no greater than 0.2 mm, aligned parallel with one another at an inclined angle to the rotational axis. The screw thread in the apical section is in form of a macrothread, having a height greater than 0.2 mm, and in case of more than one macrothread, all macrothreads are also aligned parallel with one another, at an angle inclined to the rotational axis. The pitch of the screw thread of the apical section is the same as that of the coronal section. The

quantity of the macrothreads in the apical section is less than that of the microthreads in the coronal section.

US Patent Application Publication No. 2005/0276676 A1, to Mardinger et al., and entitled "Orthopedic or Dental Device", is directed to a dental device having a screw thread whose feature is variable along the length of the dental device. These features include the spacing between adjacent turns of the thread, the height of the thread, and the thickness of the thread. The feature can vary either continuously, or in an abrupt manner. A segment of the screw thread having widely spaced turns is meant to be inserted into a cancellous bone tissue, while another segment of the screw thread having narrowly spaced turns is meant to be inserted into compact bone tissue.

U.S. Pat. No. 6,030,162 issued to Huebner and entitled "Axial Tension Screw" is directed to a screw having a leading section, an intermediate section, a trailing section, and a self drilling tip. The screw thread of the leading section has a constant pitch. The screw thread of the trailing section has a constant but smaller pitch, and the screw thread of the intermediate section has a variable pitch connecting the leading section and the trailing section.

U.S. Pat. No. 5,427,527 issued to Niznick et al., and entitled "Dental Implant Method of Installation", is directed to a cylindrical threaded implant. The implant has an angled abutment at a top portion thereof. The threads of the implant are interrupted by a plurality of closely spaced longitudinal channels, to provide a serrated appearance.

SUMMARY OF THE INVENTION

It is an object of the disclosed technique to provide a novel dental implant for attaching a tooth to a jawbone, and a method for implanting the dental implant in the jawbone.

In accordance with the disclosed technique, there is thus provided a dental implant for implanting a tooth in a jawbone. The dental implant includes a coarsely threaded portion suitable for nesting within the entire width of the cortical bone of the jawbone, and within a small portion of the cancellous bone of the jawbone. The dental implant further includes a finely threaded portion suitable for nesting within the cancellous bone of the jawbone. A primary thread runs along both the finely threaded portion and the coarsely threaded portion. The primary thread has a constant pitch and a constant major diameter, a large thread height in the coarsely threaded portion, and a small thread height in the finely threaded portion.

The small thread height is substantially greater than the height of a microthread, and the large thread height is larger than the small thread height. The primary thread has a primary thread angle more acute than 45 degrees. The dental implant further includes at least one secondary thread having the constant pitch and the small thread height, which runs along the finely threaded portion, at an offset from the primary thread. The at least one secondary thread has a secondary thread angle more acute than 45 degrees.

According to another aspect of the disclosed technique, there is thus provided a method for implanting a dental implant in a jawbone of a patient. The method includes the procedures of drilling a first bore in the jawbone, inserting a guide pin into the first bore, drilling a second bore through the cortical bone, removing the guide pin from the jawbone, and screwing the dental implant into the jawbone.

The first bore passes through a cortical bone and a cancellous bone of the jawbone. The first bore has a first diameter. The first diameter matches a small minor diameter of a coarsely threaded dental implant distal portion of the dental implant. A bore length of the first bore matches a dental

implant length of the dental implant. A bore distal part of the first bore is dedicated for tapping of the dental implant distal portion in the cancellous bone.

The second bore partially penetrates the cancellous bone, and it is drilled by employing a guided drill bit which employs the guide pin as a drilling guide. The second bore has a second diameter larger than the first diameter. The second diameter matches a large minor diameter of a finely threaded dental implant proximal portion of the dental implant. The second bore is dedicated for tapping the dental implant proximal portion.

BRIEF DESCRIPTION OF THE DRAWINGS

The disclosed technique will be understood and appreciated more fully from the following detailed description taken in conjunction with the drawings in which:

FIG. 1 is a schematic illustration of a dental implant, constructed and operative according to an embodiment of the disclosed technique;

FIG. 2 is a schematic illustration of a side view (view I) of the dental implant of FIG. 1;

FIG. 3 is a schematic illustration of a longitudinal section (section II-II) of the dental implant of FIG. 1;

FIG. 4 is a schematic illustration of a perspective view of the dental implant of FIG. 1;

FIG. 5A is a schematic illustration of a portion of a mandible in which a bore is drilled, for tapping therein the dental implant of FIG. 1;

FIG. 5B is a schematic illustration of the mandible of FIG. 5A, which includes a guide pin inserted into the bore illustrated in FIG. 5A;

FIG. 5C is a schematic illustration of the mandible of FIG. 5B, in which another bore is drilled for tapping the secondary threads of the dental implant of FIG. 1, in a cortical bone of the mandible;

FIG. 5D is a schematic illustration of the mandible of FIG. 5A, ready for tapping therein the dental implant of FIG. 1;

FIG. 6 is a schematic illustration of a drill bit employed for drilling the bore in the mandible of FIG. 5C, for tapping the secondary threads of FIG. 1, therein;

FIG. 7 is a schematic illustration of a side view (view III) of the drill bit of FIG. 6;

FIG. 8 is a schematic illustration of a section (section IV-IV) of the drill bit of FIG. 7; and

FIG. 9 is a schematic illustration of a method for implanting the dental implant of FIG. 1, into a jawbone of a patient, operative according to another embodiment of the disclosed technique.

DETAILED DESCRIPTION OF THE EMBODIMENTS

The disclosed technique overcomes the disadvantages of the prior art by providing a dental implant which includes a coarsely threaded portion and a finely threaded portion, on the dental implant. The dental implant includes a primary thread, and one or more secondary threads. The primary thread runs along the finely threaded portion and the coarsely threaded portion. The primary thread has a constant pitch and a constant major diameter. A minor diameter of the primary thread in the coarsely threaded portion is smaller than that of each of the secondary threads. Accordingly, the thread height of the primary thread in the coarsely threaded portion is larger than the thread height of either of the secondary threads or of the primary thread, in the finely threaded portion.

The pitch of each of the secondary threads is the same as that of the primary thread. Each of the secondary threads runs along the finely threaded portion, at an offset from the primary thread, equal to the value of the pitch of the primary thread, divided by the quantity of the secondary threads, plus one.

Preferably, a thread angle of each of the secondary threads is the same as that of the primary thread. The primary thread is dedicated for being tapped in both the cortical bone and the cancellous bone (i.e., a spongy region of the jawbone), and each of the secondary threads is dedicated for being tapped mainly in the cortical bone. The screw strength of a screw is proportional to the screw thread stress area of the screw. Since the minor diameter of the primary thread is smaller than that of each of the secondary threads, the screw strength of the coarsely threaded portion of the dental implant according to the disclosed technique, is greater than that of a dental implant in which the minor diameter of the coarsely threaded portion, is the same as that of the finely threaded portion. The term "thread height" herein below, refers to half the difference between a major diameter of a screw thread, and a minor diameter of the screw thread.

Reference is now made to FIGS. 1, 2, 3, and 4. FIG. 1 is a schematic illustration of a dental implant generally referenced 100, constructed and operative according to an embodiment of the disclosed technique. FIG. 2 is a schematic illustration of a side view (view I) of the dental implant of FIG. 1. FIG. 3 is a schematic illustration of a longitudinal section (section II-II) of the dental implant of FIG. 1. FIG. 4 is a schematic illustration of a perspective view of the dental implant of FIG. 1.

With reference to FIGS. 1 and 3, dental implant 100 includes a finely threaded portion 110 (i.e., finely threaded dental implant proximal portion), and a coarsely threaded portion 112 (i.e., coarsely threaded dental implant distal portion). Finely threaded portion 110 is proximal to the outer part of the jawbone, where an artificial tooth (not shown) is to be coupled to. Coarsely threaded portion 112 is at a distal end of dental implant 100. Finely threaded portion 110 is between 5 to 6.5 mm long, and coarsely threaded portion 112 is between 6.5 to 8 mm long, correspondingly, such that dental implant 100 is approximately 13 mm long.

Coarsely threaded portion 112 includes a distal end 102, which is an optional feature in form of a truncated cone tapering at an angle of α , in order to facilitate self tapping of dental implant 100 into a jawbone (not shown) of a patient (not shown). The screw thread along coarsely threaded portion 112 continues up to distal end 102. Distal end 102 is particularly short in order to avoid reduction of bonding area when dental implant 100 is subject to dislodging forces, and can be entirely eliminated, if such self tapping facilitation is redundant.

Finely threaded portion 110 has a minor diameter D_3 (FIG. 3), which is greater than a minor diameter D_2 of coarsely threaded portion 112. A proximal end 106 of dental implant 100 includes a proximal surface 108, a countersink 126, a hexagonal socket 128, and a bore 130. Bore 130 includes a top surface 132 and a bottom surface 134. Countersink 126 is located at proximal surface 108, and on the top of hexagonal socket 128. A portion of bore 130 includes an internal thread 136 running from top surface 132 toward bottom surface 134. Bore 130 is generally disposed within finely threaded portion 110.

A depth of countersink 126 is referenced h_1 . A socket depth of hexagonal socket 128 from proximal surface 108, is referenced h_2 . An opening between every two internal surfaces of hexagonal socket 128, is referenced d_2 (FIG. 2). A depth of

5

bore 130 from top surface 132 to bottom surface 134 is referenced h_3 . A distance between proximal surface 108 to bottom surface 134 is referenced h_4 . A diameter of bore 130 is referenced d_1 .

A dental surgeon (not shown) screws dental implant 100 into the jawbone, by employing a mounting device (e.g., an Allen wrench—not shown), which fits hexagonal socket 128. A major diameter (not shown) of internal thread 136 is such that a wall thickness (not shown) between internal thread 136 and minor diameter D_3 , is of such a value that the strength of dental implant 100 is not compromised. Alternatively, bore 130 can extend within coarsely threaded portion 112, if the diameter (not shown) of bore 130 and is smaller than minor diameter D_2 such that wall thickness (not shown) between bore 130 (or internal thread 136) and minor diameter D_2 , is of such a value that the strength of dental implant 100 is not compromised. It is noted that the screw thread of finely threaded portion 110 can extend up to proximal surface 108.

After implanting dental implant 100 within the jawbone, the dental surgeon screws a flat head screw (not shown), in internal thread 136, and sutures the wound in the jawbone. The head of the flat head screw fits countersink 126, thereby positively sealing hexagonal socket 128 during the healing period. When the jawbone grows, the dental surgeon removes the flat head screw, and mounts an artificial tooth (not shown) on proximal end 106. The dental surgeon can mount the artificial tooth on dental implant 100, by screwing an external threaded portion of the artificial tooth, into internal thread 136. Alternatively, the dental surgeon can mount the artificial tooth on dental implant 100, by applying an adhesive between the artificial tooth and hexagonal socket 128 or bore 130.

The mounting device may further include a pin that enters bores 130, for imparting rigidity between the mounting device and dental implant 100. In order to prevent contamination, the manufacturer of dental implant 100, can pack dental implant 100 together with the mounting device, in an sterilized enclosure. In this case, throughout the operation, the dental surgeon comes in contact only with the mounting device, and discards the mounting device after implanting dental implant 100 in the jawbone. In this case, hand contact with dental implant 100 is prevented.

Dental implant 100 is of a length L_1 and includes finely threaded portion 110 of a length L_2 and coarsely threaded portion 112 of a length L_3 . Dental implant 100 further includes a primary thread 114 and one or more secondary threads 116. Primary thread 114 runs seamlessly along the entire length of dental implant 100, namely—along both finely threaded portion 110 and coarsely threaded portion 112. Primary thread 114 has a constant pitch P , and a major diameter D_1 . The value of major diameter D_1 is between 3.75 and 4.6 mm. The value of constant pitch P is between 1 and 1.3 mm. Primary thread 114 has a large thread height (not shown) in coarsely threaded portion 112, and a small thread height (not shown) in finely threaded portion 110, wherein the large thread height is larger than the small thread height. The value of the small thread height is between 0.4 and 0.7 mm. The value of the large thread height is between 1 and 1.4 mm.

The large thread height defines a small minor diameter D_2 respective of primary thread 114. The small thread height defines a large minor diameter D_3 respective of each of secondary threads 116, wherein

$$D_3 > D_2 \quad (1)$$

It is noted that the greater the difference between major diameter D_1 and each of minor diameters D_2 and D_3 , respectively, the greater is the thread height and the greater is the contact surface between dental implant 100 and the jawbone. This

6

substantially large contact surface, has a significant role in resisting the tensile forces and the moments, which act on dental implant 100 especially during mastication. Therefore, this contact surface should be as large as possible.

In order to avoid moments and tensile forces which can damage dental implant 100 during the screwing operation within the jawbone, the pitch of each of secondary threads 116, substantially equals to pitch P of primary thread 114. Each of secondary threads 116 runs in parallel to the primary thread 114, along finely threaded portion 110, at an offset. This offset equals to $P/(n+1)$, where $n=1, 2, 3 \dots N$ is the quantity of the secondary threads 116, which are manufactured in finely threaded portion 110. In case there is only one secondary thread 116, $n=1$, and the offset equals to half of the pitch P .

Preferably, a thread angle β of primary thread 114 (i.e., primary thread angle) is substantially the same as that of each of secondary threads 116 (i.e., secondary thread angle), although the primary thread angle and the secondary thread angle can be different. Each of the primary thread angle and the secondary thread angle is an acute angle of less than 45 degrees, and preferably 30 degrees. Primary thread 114 is represented by a plurality of crests 118. Each of secondary threads 116 is represented by a plurality of crests 120. The distance between every adjacent pair of crests 120 and 118 along a longitudinal axis 122 of dental implant 100, substantially equals to $P/2$. Secondary thread 116 ends with an intermediate screw turn 124, whose major diameter gradually reduces from D_1 to D_3 . Alternatively, the major diameter of intermediate screw reduces from D_1 to D_2 .

A jawbone (i.e., either the mandible or maxilla) of a human being includes a cortical bone below the gingiva, and a cancellous (spongy) bone below the cortical bone. The cortical bone is a substantially compact and solid bone, whereas the cancellous bone is porous and includes voids (similar to a sponge), and is not as strong as the cortical bone. Therefore, when a screw is tapped into the cortical bone and the cancellous bone of the jawbone, an upper portion of the screw which is located in the cortical bone, provides significant bonding that carries most of the load, while the lower portion of the screw which is located in the cancellous bone provides bonding of lesser significance.

The proof strength of a bolt which is tightened into a nut, in terms of tension and torque, is proportional to the stress area (i.e., the total surface area of those screw threads of the bolt which are in contact with the screw threads of the nut). Therefore, the greater the stress area, the greater the tensile load and the torque which the bolt can carry. The disclosed technique employs a screw whose coarsely threaded portion 112, which is located in the cancellous bone, has a stress area which is greater than that of finely threaded portion 110, which is located in the cortical bone. As the dental surgeon screws dental implant 100 into the jawbone, dental implant 100 compresses the cancellous bone surrounding the coarsely threaded portion of dental implant 100, thus strengthening the anchoring of dental implant 100 to the jawbone and expediting bone growth around dental implant 100. Therefore, the screw thread profile according to the disclosed technique provides a dental implant which has a proof strength substantially greater than that of a dental implant whose screw thread is uniform.

According to (1), minor diameter D_2 is smaller than minor diameter D_3 . Therefore, the stress area of coarsely threaded portion 112 is greater than that of finely threaded portion 110. It is noted that the large thread height of primary thread 114 is larger than that of each of secondary threads 116. It is further noted, that since the pitch of primary thread 114 is substan-

tially the same as that of each of secondary threads **116**, after tapping a thread in the cortical bone by primary thread **114**, each of secondary threads **116** carves and thus taps into a screw thread in parallel to the one formed by primary thread **114**, in the cortical bone.

Dental implant **100** can include one or more longitudinal grooves (not shown), on a periphery thereof, disposed along longitudinal axis **122**. Each of the longitudinal grooves can be located either on primary thread **114**, each of secondary threads **116**, or both primary thread **114** and secondary threads **116**. While the dental surgeon screws dental implant **100** into the jawbone, bone particles which are produced due to the screwing action of primary thread **114** and secondary threads **116** into the jawbone, are deposited in the longitudinal grooves. In this manner, the longitudinal grooves serves as a depository for the bone particles. During the healing process, bone cells grow into the longitudinal grooves. Therefore, the longitudinal grooves provide an anchoring function in addition to that provided by primary thread **114** and secondary threads **116**.

Reference is now made to FIGS. **5A**, **5B**, **5C**, **5D**, **6**, **7**, and **8**. FIG. **5A** is a schematic illustration of a portion of a mandible in which a bore is drilled, for tapping the dental implant of FIG. **1**, therein. FIG. **5B** is a schematic illustration of the mandible of FIG. **5A**, which includes a guide pin inserted into the bore illustrated in FIG. **5A**. FIG. **5C** is a schematic illustration of the mandible of FIG. **5B**, in which another bore is drilled for tapping the secondary threads of the dental implant of FIG. **1**, in a cortical bone of the mandible. FIG. **5D** is a schematic illustration of the mandible of FIG. **5A**, ready for tapping the dental implant of FIG. **1**, therein. FIG. **6** is a schematic illustration of a drill bit employed for drilling the bore in the mandible of FIG. **5C**, for tapping the secondary threads of FIG. **1**, therein. FIG. **7** is a schematic illustration of a side view (view III) of the drill bit of FIG. **6**. FIG. **8** is a schematic illustration of a section (section IV-IV) of the drill bit of FIG. **7**.

With reference to FIG. **5A**, a mandible **200** includes a cortical bone **202** and a cancellous bone **204**. Cortical bone **202** is covered by a gingiva **206**. A thickness of cortical bone **202** is designated by L_4 . A bore **208**, of a diameter D_4 , is drilled to a depth L_1 (FIG. **1**), from a crest line **212** into cortical bone **202** and cancellous bone **204**.

With reference to FIG. **5B**, a guide pin **210**, of a length L_5 , longer than the length L_1 (FIG. **1**) of dental implant **100** (i.e., depth L_1 is the same as the length of dental implant **100**), and a diameter D_5 , is inserted into bore **208**. Preferably, length L_5 of guide pin **210**, is longer than L_1 , by 3 mm. Diameter D_5 of guide pin **210** is equal to or greater than diameter D_4 (FIG. **5A**) of bore **208**. Guide pin **210** is made of a metal, such as stainless steel, titanium, and the like. Guide pin **210** protrudes from crest line **212** by a length L_6 .

With reference to FIGS. **5C**, **5D**, **6**, **7**, and **8**, a bore **230** of a diameter D_6 , is drilled through cortical bone **202** and slightly penetrates cancellous bone **204**, to a depth L_4 (FIG. **5D**) from crest line **212**, by employing a guided drill bit **214** (FIG. **6**), while guide pin **210** is located within bore **208** (FIG. **5A**). Depth L_4 is greater than the thickness of cortical bone **202**. Considering the diversity of the thickness of cortical bone **202** among different patients, by selecting a typical value of 5 mm for L_4 , total penetration of finely threaded portion **110** through all of cortical bone **202**, as well as slight penetration into cancellous bone **204**, is provided.

Guided drill bit **214** (FIG. **6**) includes a shank **216** and a cutting portion **218**. Shank **216** is employed for attaching guided drill bit **214** to a drill (not shown). Shank **216** includes an inlet cooling channel **220**. Cutting portion **218** has a diam-

eter D_6 (FIGS. **6** and **5D**). Cutting portion **218** includes a plurality of outlet cooling holes **222** in a periphery thereof. Cutting portion **218** includes a bore **224** to fit guide pin **210** (FIG. **5B**). Bore **224** has a diameter D_7 larger than D_5 (FIG. **5B**) of guide pin **210**. Bore **224** has a depth $L_7=L_4+L_6$.

While guide pin **210** is located within mandible **200**, the dental surgeon uses guided drill bit **214** to drill bore **230** of diameter D_6 through cortical bone **202** into cancellous bone **204**, by employing guide pin **210** as a pilot bit. When a bottom portion **226** (FIG. **8**) of bore **224** makes contact with an end **228** (FIG. **5B**) of guide pin **210**, guided drill bit **214** ceases to advance any further into mandible **200**. In this manner, bore **230** is drilled into cortical bone **202**, to depth L_4 (FIG. **5C**) from crest line **212**. Inlet cooling channel **220** is in fluid communication with outlet cooling holes **222**, in order to allow a cooling fluid to flow from inlet cooling channel **220** to hole **224**, and out through outlet cooling holes **222**.

With reference to FIG. **5D**, after removing guide pin **210** and guided drill bit **214** from mandible **200**, bore **230** of diameter D_6 to the depth of L_4 from crest line **212**, is drilled through cortical bone **202**, while slightly penetrating cancellous bone **204**. The remainder of bore **208** is located within cancellous bone **204** from below cortical bone **202**, having a depth L_3 . The value of diameter D_4 (FIG. **5D**) of bore **208** is selected according to the value of minor diameter D_2 (FIG. **3**) of primary thread **114**, such that primary thread **114** can be self tapped into bore **208** of cancellous bone **204**. Similarly, the value of diameter D_6 of bore **230** is selected according to the value of minor diameter D_3 of each of secondary threads **116**, in order to provide self tapping of each of secondary threads **116**, into bore **230** of cortical bone **202**.

The small thread height is substantially greater than the height of a micro thread, namely, substantially more than 0.2 mm. Preferably, the small thread height should be between 0.4 mm to 0.7 mm, and most preferably approximately 0.5 mm.

The values of the parameters of dental implant **100** can be for example, as follows:

- $L_1=13$ mm
- $L_2=6.3$ mm
- $L_3=6.7$ mm
- $P=1.2$ mm
- $\alpha=45^\circ$
- $\beta=30^\circ$
- $D_1=4.5$ mm
- $D_2=1.9$ mm
- $D_3=3.5$ mm
- small thread height=0.5 mm $(=(D_1-D_3)/2)$
- large thread height=0.5 mm $(=(D_1-D_2)/2)$

Some of the parameters of dental implant **100** at proximal end **106** are for example, as follows:

- $h_1=0.4$ mm
- $h_2=2.6$ mm
- $h_3=3.7$ mm
- $h_4=6.3$ mm
- $d_1=1.3$ mm
- $d_2=2.6$ mm

The values of the parameters of complementary drilling method and apparatus can be for example, as follows:

- $D_4=D_5=D_2=1.9$ mm
- $D_6=3.5$ mm
- $D_7=2.1$ mm
- $L_4=L_2=6.3$ mm
- $L_5=16$ mm
- $L_6=3$ mm
- $L_7=9.3$ mm

9

Reference is now made to FIG. 9, which is a schematic illustration of a method for implanting the dental implant of FIG. 1, into a jawbone of a patient, operative according to another embodiment of the disclosed technique. In procedure 250, a first bore is drilled in a jawbone of a patient, the first bore passing through a cortical bone and a cancellous bone of the jawbone. The first bore has a first diameter matching a small minor diameter of a coarsely threaded dental implant portion of a dental implant. A bore length of the first bore matches a dental implant length of the dental implant. A bore distal part of the first bore is dedicated for tapping of the dental implant distal portion into the cancellous bone.

With reference to FIGS. 1 and 5A, bore 208 of diameter D_4 , is drilled into mandible 200. Bore 208 is drilled through both cortical bone 202 and cancellous bone 204.

In procedure 252, a guide pin is inserted into the first bore, the guide pin being longer than the first bore. With reference to FIG. 5B, guide pin 210 which is of a length L_5 , longer than the length L_1 of dental implant 100 by a length L_6 , is inserted into bore 208.

In procedure 254, a second bore is drilled through the cortical bone, partially penetrating the cancellous bone, by employing a guided drill bit which employs the guide pin as a drilling guide. The second bore has a second diameter larger than the first diameter. The second diameter matches a large minor diameter of a finely threaded dental implant proximal portion of the dental implant. The second bore is dedicated for tapping the dental implant proximal portion. With reference to FIGS. 1, 5C, and 5D, bore 230 of diameter D_6 , is drilled through cortical bone 202 and into cancellous bone 204, by employing guided drill bit 214, which was inserted into mandible 200, in procedure 250. Guided drill bit 214 advances within cortical bone 202 and slightly further—into the cancellous bone 204 along guide pin 210, which is located within bore 224 of guided drill bit 214.

In procedure 256, the guide pin is removed from the jawbone. With reference to FIGS. 1 and 5D, the dental surgeon removes guide pin 210 from mandible 200, and implants dental implant 100 into mandible 200, by screwing of dental implant 100 into mandible 200 (procedure 258). Primary thread 114 taps a screw thread of pitch P in bore 230 of cortical bone 202. As dental implant 100 advances further into mandible 200, dental implant 100 taps one or more secondary threads 116, into bore 230 of cortical bone 202 while primary thread 114 is further advanced into the distal portion of bore 208 into cancellous bone 204. Since the pitch of each of secondary threads 116 is the same as that of primary thread 114, each of secondary threads 116 taps into a screw thread which is parallel to the screw thread tapped in cortical bone 202 by primary thread 114 in procedure 250. Further procedures in respect with the use of a mounting device, its application for screwing dental implant 100, removal of the mounting device, sealing of dental implant 100, and the coupling of an artificial tooth into dental implant 100, are described herein above in connection with FIGS. 1 to 3.

It will be appreciated by persons skilled in the art that the disclosed technique is not limited to what has been particularly shown and described hereinabove. Rather the scope of the disclosed technique is defined only by the claims, which follow.

The invention claimed is:

1. A dental implant for attaching therewith an artificial tooth to a jawbone, the dental implant comprising:

a finely threaded portion configured for nesting within the entire width of a cortical bone of said jawbone and within a small portion of a cancellous bone of said jaw-

10

bone, said finely threaded portion having a first number of thread crests per axial distance; and

a coarsely threaded portion configured for nesting within said cancellous bone, said coarsely threaded portion having a second number of thread crests per axial distance, lesser than said first number of thread crests per axial distance,

said dental implant including a plurality of primary threads running along both said finely threaded portion and said coarsely threaded portion, and one or more secondary threads running along said finely threaded portion at an offset from said primary threads, said offset is based on a number of said one or more secondary threads in said finely threaded portion,

wherein the thread crests of the coarsely threaded portion are formed by said plurality of primary threads in the coarsely threaded portion, and the thread crests of the finely threaded portion are formed by the plurality of primary threads and the one or more secondary threads in the finely threaded portion,

wherein the primary threads having a constant pitch and a constant major diameter throughout both said finely threaded portion and said coarsely threaded portion,

said primary threads comprising a larger thread height in said coarsely threaded portion and a smaller thread height, lesser than said larger thread height, in said finely threaded portion,

said primary threads comprising a larger minor diameter in said coarsely threaded portion and a smaller minor diameter, lesser than said larger minor diameter, in said finely threaded portion,

wherein the secondary threads have constant pitch, wherein said smaller thread height is between 0.2 millimeter and 0.7 millimeter,

wherein said larger thread height is between 1 and 1.4 millimeters,

and wherein said constant major diameter is between 3.75 and 4.6 millimeters.

2. The dental implant according to claim 1, wherein said offset is based on $P/(n+1)$, where “ n ” is equal to the number of said one or more secondary threads in said finely threaded portion, and “ P ” is the pitch of said primary threads.

3. The dental implant according to claim 1, wherein the value of said smaller thread height is between 0.4 and 0.7 millimeter.

4. The dental implant according to claim 3, wherein the value of said smaller thread height is 0.5 millimeter.

5. The dental implant according to claim 1, wherein the value of said larger thread height is 1.3 millimeters.

6. The dental implant according to claim 1, wherein said primary threads comprising a primary thread angle more acute than 45 degrees, and said secondary threads comprising a secondary thread angle more acute than 45 degrees.

7. The dental implant of claim 6, wherein the value of at least one of said primary thread angle and said secondary thread angle is 30 degrees.

8. The dental implant according to claim 1, wherein the value of said constant major diameter is 4.5 millimeters.

9. The dental implant according to claim 1, wherein the value of said constant pitch is between 1 and 1.3 millimeters.

10. The dental implant according to claim 1, wherein the value of said constant pitch is 1.2 millimeters.

11. The dental implant according to claim 1, wherein said finely threaded portion is between 5 to 6.5 millimeters long, and said coarsely threaded portion is between 6.5 to 8 millimeters long.

11

12. The dental implant according to claim **11**, wherein said finely threaded portion is 6.3 millimeters long, and said coarsely threaded portion is 6.7 millimeters long.

13. The dental implant of claim **1**, wherein a ratio between said larger thread height and said smaller thread height is between 2 to 2.5.

* * * * *

12