

US008506558B2

(12) **United States Patent**  
**Gertner et al.**

(10) **Patent No.:** **US 8,506,558 B2**  
(45) **Date of Patent:** **\*Aug. 13, 2013**

(54) **SYSTEM AND METHOD FOR PERFORMING AN OCULAR IRRADIATION PROCEDURE**

(75) Inventors: **Michael Gertner**, Menlo Park, CA (US); **Mark Arnoldussen**, San Carlos, CA (US); **Matt Herron**, Palo Alto, CA (US)

(73) Assignee: **Oraya Therapeutics, Inc.**, Newark, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1387 days.  
This patent is subject to a terminal disclaimer.

(21) Appl. No.: **12/027,069**

(22) Filed: **Feb. 6, 2008**

(65) **Prior Publication Data**

US 2009/0182310 A1 Jul. 16, 2009

**Related U.S. Application Data**

(60) Provisional application No. 61/020,655, filed on Jan. 11, 2008.

(51) **Int. Cl.**  
**A61F 9/007** (2006.01)  
**A61B 18/18** (2006.01)  
**A61N 5/01** (2006.01)

(52) **U.S. Cl.**  
USPC ..... **606/4; 606/12; 378/65**

(58) **Field of Classification Search**  
None  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,073,960 A 1/1963 Guentner et al.  
4,391,275 A 7/1983 Fankhauser et al.  
4,521,905 A 6/1985 Hosokawa  
4,710,193 A 12/1987 Volk  
4,718,418 A 1/1988 L'Esperance, Jr.  
4,817,432 A 4/1989 Wallace et al.  
5,008,907 A 4/1991 Norman et al.  
5,027,818 A 7/1991 Bova et al.  
5,065,031 A 11/1991 Moscovitch  
5,116,115 A 5/1992 Lange et al.  
5,139,494 A 8/1992 Freiberg  
5,171,254 A 12/1992 Sher  
5,189,687 A 2/1993 Bova et al.  
5,207,223 A 5/1993 Adler  
5,216,255 A 6/1993 Weidlich  
5,304,167 A 4/1994 Freiberg  
5,336,215 A \* 8/1994 Hsueh et al. .... 606/4  
5,339,347 A 8/1994 Slatkin et al.  
5,354,323 A 10/1994 Whitebook  
5,373,844 A 12/1994 Smith et al.  
5,411,026 A 5/1995 Carol  
5,422,926 A 6/1995 Smith et al.  
5,427,097 A 6/1995 Depp  
5,430,308 A 7/1995 Feichtner et al.  
5,446,548 A 8/1995 Gerig et al.

5,468,238 A 11/1995 Mersch  
5,528,652 A 6/1996 Smith et al.  
5,556,417 A 9/1996 Sher  
5,635,721 A 6/1997 Bardi et al.  
5,644,616 A 7/1997 Landi et al.  
5,651,043 A 7/1997 Tsuyuki et al.  
5,668,847 A 9/1997 Hernandez  
5,708,696 A 1/1998 Kantor  
5,724,400 A 3/1998 Swerdloff et al.  
5,727,042 A 3/1998 Brenneisen  
5,737,384 A 4/1998 Fenn  
5,744,919 A 4/1998 Mishin et al.  
5,745,545 A 4/1998 Hughes  
5,771,270 A 6/1998 Archer  
5,778,043 A 7/1998 Cosman  
5,820,553 A 10/1998 Hughes  
5,870,697 A 2/1999 Chandler et al.  
5,901,199 A 5/1999 Murphy et al.  
6,001,054 A 12/1999 Regulla et al.  
6,104,778 A 8/2000 Murad  
6,126,668 A 10/2000 Bair et al.  
6,134,294 A \* 10/2000 Gibbs ..... 378/65

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 2152145 A1 2/2010  
EP 2231277 A1 9/2010

(Continued)

**OTHER PUBLICATIONS**

International Search Report and Written Opinion for PCT/US2008/012341, search report dated Feb. 5, 2009, 21 pages (2009).  
Cornsweet, T.N. and Crane, H.D., "Accurate Two-Dimensional Eye Tracker Using First and Fourth Purkinje", *Journal of the Optical Society of America*, 63(8):921-928 (1973).  
Das et al., "Small Fields: Nonequilibrium Radiation Dosimetry", *Medical Physics*, 35(1):206-215 (2008).  
Esquivel, Carlos Jr. et al., Novel low-kVp beamlet system for choroidal melanoma, *Radiation Oncology*, I:36, 12 pages (2006).  
Fakiris, Achilles J. et al., Gamma-Knife-Based Stereotactic Radiosurgery for Uveal Melanoma, *Stereotactic and Functional Neurosurgery*, 85:106-112 (2007).

(Continued)

*Primary Examiner* — Robert A. Wax  
*Assistant Examiner* — H. Sarah Park  
(74) *Attorney, Agent, or Firm* — James W. Hill; M. Todd Hales; McDermott Will & Emery LLP

(57) **ABSTRACT**

A method and system for performing an ocular irradiation procedure on a patient's eye is disclosed. The system includes a head support for supporting the patient's head, an eye-contact device attachable to the front portion of the patient's eye, to stabilize the position of the eye; and a position detector for determining the position of the contact device in the external coordinate system. A source of a collimated electromagnetic radiation beam in the system is controlled by a beam-positioning assembly for positioning the beam source such that the beam, when activated, is aimed along a selected path at a selected coordinate in the external coordinate system corresponding to a selected target region in the patient's eye.

**14 Claims, 17 Drawing Sheets**



2006/0067469 A1 3/2006 Dooley et al.  
 2006/0072821 A1 4/2006 Wang  
 2006/0074292 A1 4/2006 Thomson et al.  
 2006/0074299 A1 4/2006 Sayeh  
 2006/0074304 A1 4/2006 Sayeh  
 2006/0078087 A1 4/2006 Forman et al.  
 2006/0084952 A1 4/2006 Pallikaris et al.  
 2006/0093089 A1 5/2006 Vertatschitsch et al.  
 2006/0170679 A1 8/2006 Wang et al.  
 2006/0170865 A1 8/2006 Hirohara et al.  
 2006/0176997 A1 8/2006 Dilmanian et al.  
 2006/0182326 A1 8/2006 Schildkraut et al.  
 2006/0192921 A1\* 8/2006 Loesel et al. .... 351/219  
 2006/0193441 A1 8/2006 Cadman  
 2006/0199991 A1 9/2006 Lewis et al.  
 2006/0203964 A1 9/2006 Nyholm et al.  
 2006/0245543 A1 11/2006 Earnst et al.  
 2006/0271025 A1\* 11/2006 Jones et al. .... 606/4  
 2006/0274061 A1 12/2006 Wang et al.  
 2006/0274885 A1 12/2006 Wang et al.  
 2006/0274924 A1 12/2006 West et al.  
 2006/0274925 A1 12/2006 West et al.  
 2006/0285641 A1 12/2006 Scherch  
 2006/0287662 A1 12/2006 Berry et al.  
 2006/0291621 A1 12/2006 Yan et al.  
 2006/0291710 A1 12/2006 Wang et al.  
 2006/0293583 A1 12/2006 Saracen et al.  
 2007/0003007 A1 1/2007 Carrano et al.  
 2007/0003123 A1 1/2007 Fu et al.  
 2007/0015991 A1 1/2007 Fu et al.  
 2007/0038058 A1 2/2007 West et al.  
 2007/0053490 A1 3/2007 Wang et al.  
 2007/0053491 A1 3/2007 Schildkraut et al.  
 2007/0071168 A1 3/2007 Allison et al.  
 2007/0071176 A1 3/2007 Main et al.  
 2007/0078306 A1 4/2007 Allison et al.  
 2007/0083087 A1 4/2007 Carda  
 2007/0093795 A1 4/2007 Melcher et al.  
 2007/0118010 A1 5/2007 Hillstead et al.  
 2007/0127622 A1 6/2007 Main et al.  
 2007/0127845 A1 6/2007 Fu et al.  
 2007/0140413 A1 6/2007 Saracen  
 2007/0169265 A1 7/2007 Saracen et al.  
 2007/0195929 A1 8/2007 Ruchala et al.  
 2007/0225691 A1 9/2007 Silvestrini et al.  
 2007/0225693 A1 9/2007 Muehlhoff et al.  
 2007/0249911 A1 10/2007 Simon  
 2008/0049896 A1 2/2008 Kuduvalli  
 2008/0056434 A1 3/2008 Grozinger et al.  
 2008/0159478 A1 7/2008 Keall et al.  
 2008/0187099 A1 8/2008 Gertner  
 2008/0187101 A1 8/2008 Gertner  
 2008/0192892 A1 8/2008 Dilmanian et al.  
 2008/0212737 A1 9/2008 D'Souza et al.  
 2008/0212738 A1 9/2008 Gertner  
 2008/0317312 A1 12/2008 Carl et al.  
 2009/0003525 A1 1/2009 Gertner et al.  
 2009/0163898 A1 6/2009 Gertner et al.  
 2009/0182310 A1 7/2009 Gertner et al.

FOREIGN PATENT DOCUMENTS

JP 06-181945 A 7/1994  
 JP 06-277248 A 10/1994  
 JP 2000-509291 A 7/2000  
 JP 2001-079102 A 3/2001  
 JP 2002-502647 A 1/2002  
 JP 2002-540837 A 12/2002  
 JP 2004-501730 A 1/2004  
 JP 2005-237730 A 9/2005  
 JP 2007-501057 A 1/2007  
 JP 2007-509668 A 4/2007  
 JP 4043028 B2 2/2008  
 JP 4354737 B2 10/2009  
 JP 4436139 B2 1/2010  
 JP 4602356 B2 10/2010  
 JP 5086523 B2 11/2012  
 WO 9527453 A1 10/1995  
 WO 00/59395 A1 10/2000

WO WO-0126591 A1 4/2001  
 WO WO-0235996 A1 5/2002  
 WO 03/008543 A 1/2003  
 WO WO-03/039370 A1 5/2003  
 WO 2005/016258 A2 2/2005  
 WO 2005/049139 A1 6/2005  
 WO 2005/079294 A2 9/2005  
 WO 2006/090217 A1 8/2006  
 WO WO-2006086631 A2 8/2006  
 WO WO-2007/027164 3/2007  
 WO 2007/045075 A1 4/2007  
 WO 2008/124801 A2 10/2008  
 WO 2008/0150330 A1 12/2008  
 WO 2009/075714 A1 6/2009

OTHER PUBLICATIONS

Francescon et al., "Total Scatter Factors of Small Beans: A Multidetector and Monte Carlo Study", *Medical Physics*, 35(2):504-513 (2008).  
 Georgopoulos, Michael et al., Tumour Regression of Uveal Melanoma after Ruthenium-106 Brachytherapy or Stereotactic Radiotherapy with Gamma Knife or Linear Accelerator, *Ophthalmologica*, 217:315-319 (2003).  
 Kirwan, James F. et al., Effect of  $\beta$  radiation on success of glaucoma drainage surgery in South Africa: randomized controlled trial, *BMJ online*, BMJ doi:10.1136/bmj.38971.395301.7C (Oct. 5, 2006).  
 Kishi, Kazushi et al., Lead Contact Lens for Crystalline Lens Shielding in Electron Therapy for Eyelid Tumors, *Radiation Medicine*, 14(2):107-109 (1996).  
 International Search Report and Written Opinion for PCT/US2008/013886, search report dated May 22, 2009, 19 pages (2009).  
 U.S. application and Preliminary Amendment U.S. Appl. No. 12/027,083, filed Feb. 6, 2008, 105 pages (2008).  
 U.S. application and Preliminary Amendment U.S. Appl. No. 12/027,094, filed Feb. 6, 2008, 111 pages (2008).  
 U.S. Appl. No. 12/103,534, filed Apr. 15, 2008, 99 pages (2008).  
 U.S. application and Preliminary Amendment U.S. Appl. No. 12/262,031, filed Oct. 30, 2008, 163 pages (2008).  
 U.S. Appl. No. 12/338,634, filed Dec. 18, 2008, 244 pages (2008).  
 Bogner, J. et al. 2003. A Noninvasive Eye Fixation and Computer-Aided Eye Monitoring System for Linear Accelerator-Based Stereotactic Radiotherapy of Uveal Melanoma. *International Journal of Radiation Oncology Biology Physics*, vol. 56, No. 4, Jun. 20, 2001, pp. 1128-1136.  
 Petersch, B. et al. 2004. Automatic Real-Time Surveillance of Eye Position and Gating for Stereotactic Radiotherapy of Uveal Melanoma. *Medical Physics*, vol. 31, No. 12, Nov. 24, 2004, pp. 3521-3527.  
 Extended European Search Report, dated Jun. 1, 2011, for European Patent Application No. 08743035.1, which entered the European Regional Phase on Dec. 3, 2009, Applicant Oraya Therapeutics, entitled "Device and Assembly for Positioning, Stabilizing and Treating an Eye," based on PCT Application No. PCT/US2008/004999.  
 International Search Report and Written Opinion for PCT/US2008/004999, search report dated Sep. 2, 2008, 9 pages (2008).  
 International Search Report and Written Opinion for PCT/US2008/005101, search report dated Sep. 2, 2008, 11 pages (2008).  
 Jaywant, S.E. et al., "Stereotactic Radiotherapy in the Treatment of Ocular Melanoma: A Noninvasive Eye Fixation Aid and Tracking System", *Journal of Applied Clinical Medical Physics*, 4(2):156-161 (2003).  
 Dieckmann et al., "A Linac-Based Stereotactic Irradiation Technique of Uveal Melanoma," *Radiation Therapy and Oncology*, 61:49-56 (2001).  
 Gao et al., "Orthovoltage radiation therapy treatment planning using Monte Carlo Simulation: treatment of neuroendocrine carcinoma of the maxillary sinus," ISSN: 0031-9155; vol. 42, No. 12., pp. 2421-2433 (1997).  
 Kim et al., "Combination hyperthermia and radiation therapy for malignant melanoma," *Cancer*, 50:478-482 (1982).  
 Kobayashi et al., Radiotherapy for subfoveal neovascularisation associated with pathological myopia: a pilot study., *J. Opth.* 87:761-766 (2000).

\* cited by examiner

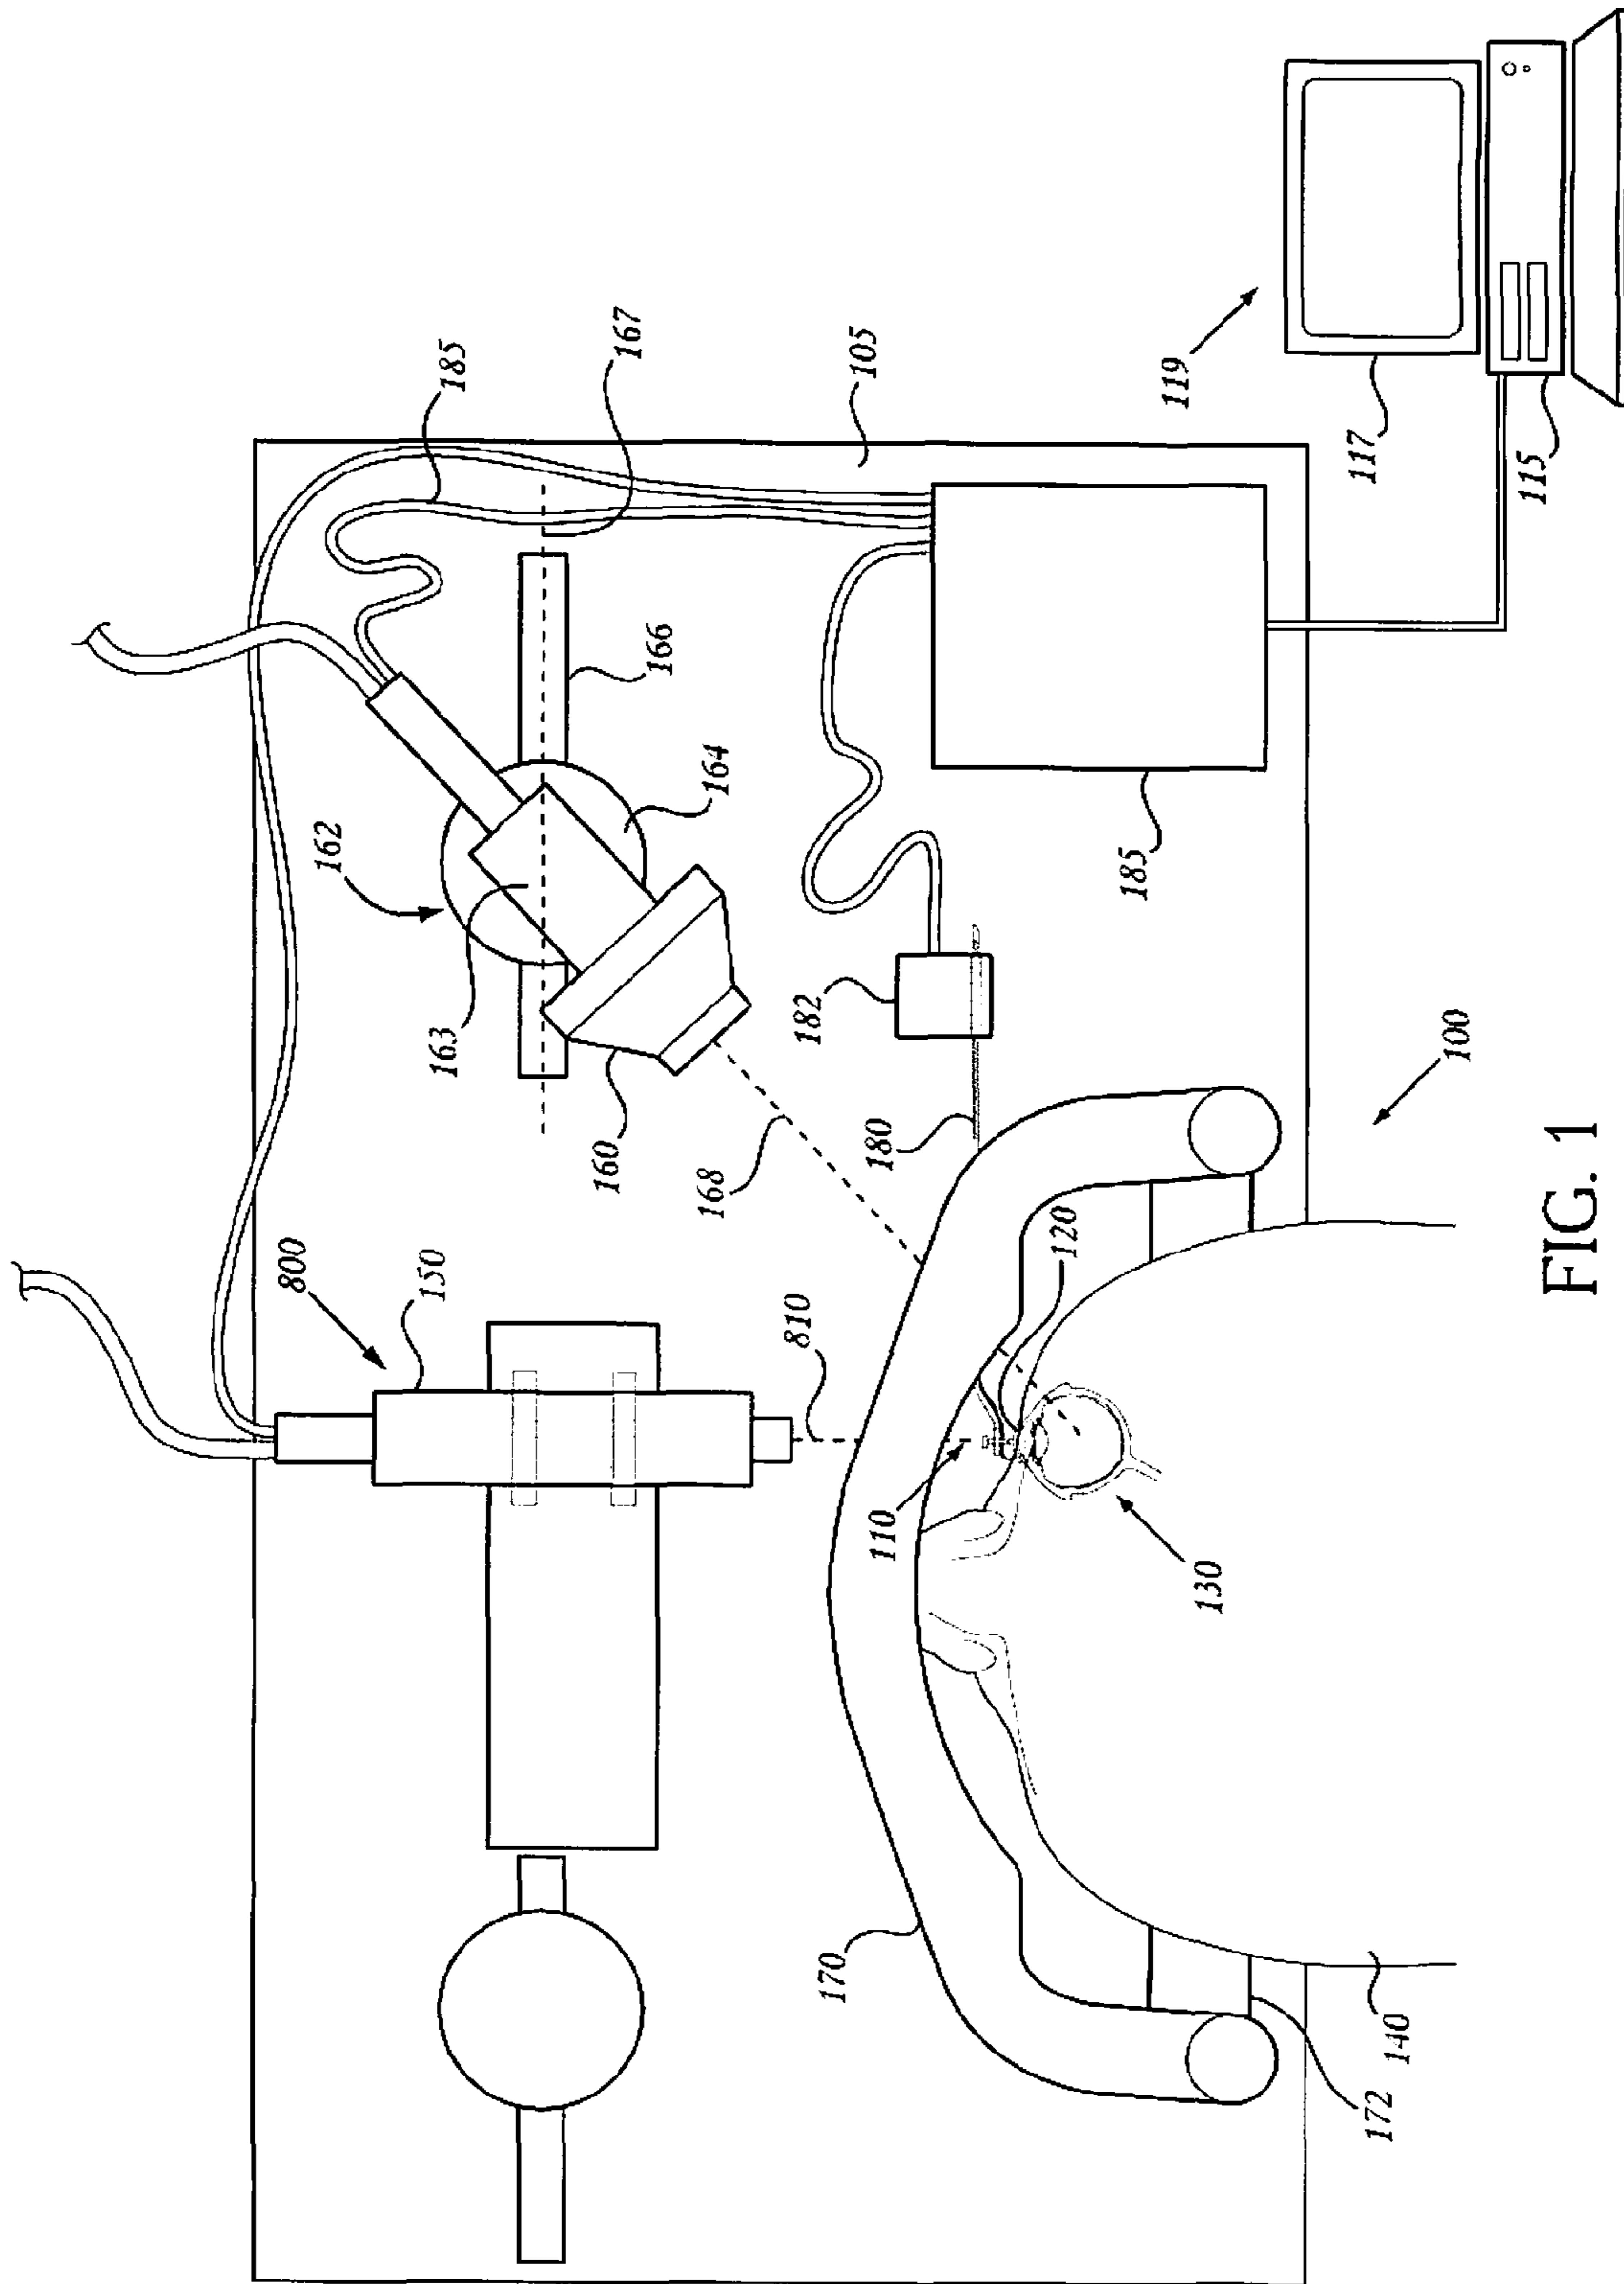


FIG. 1

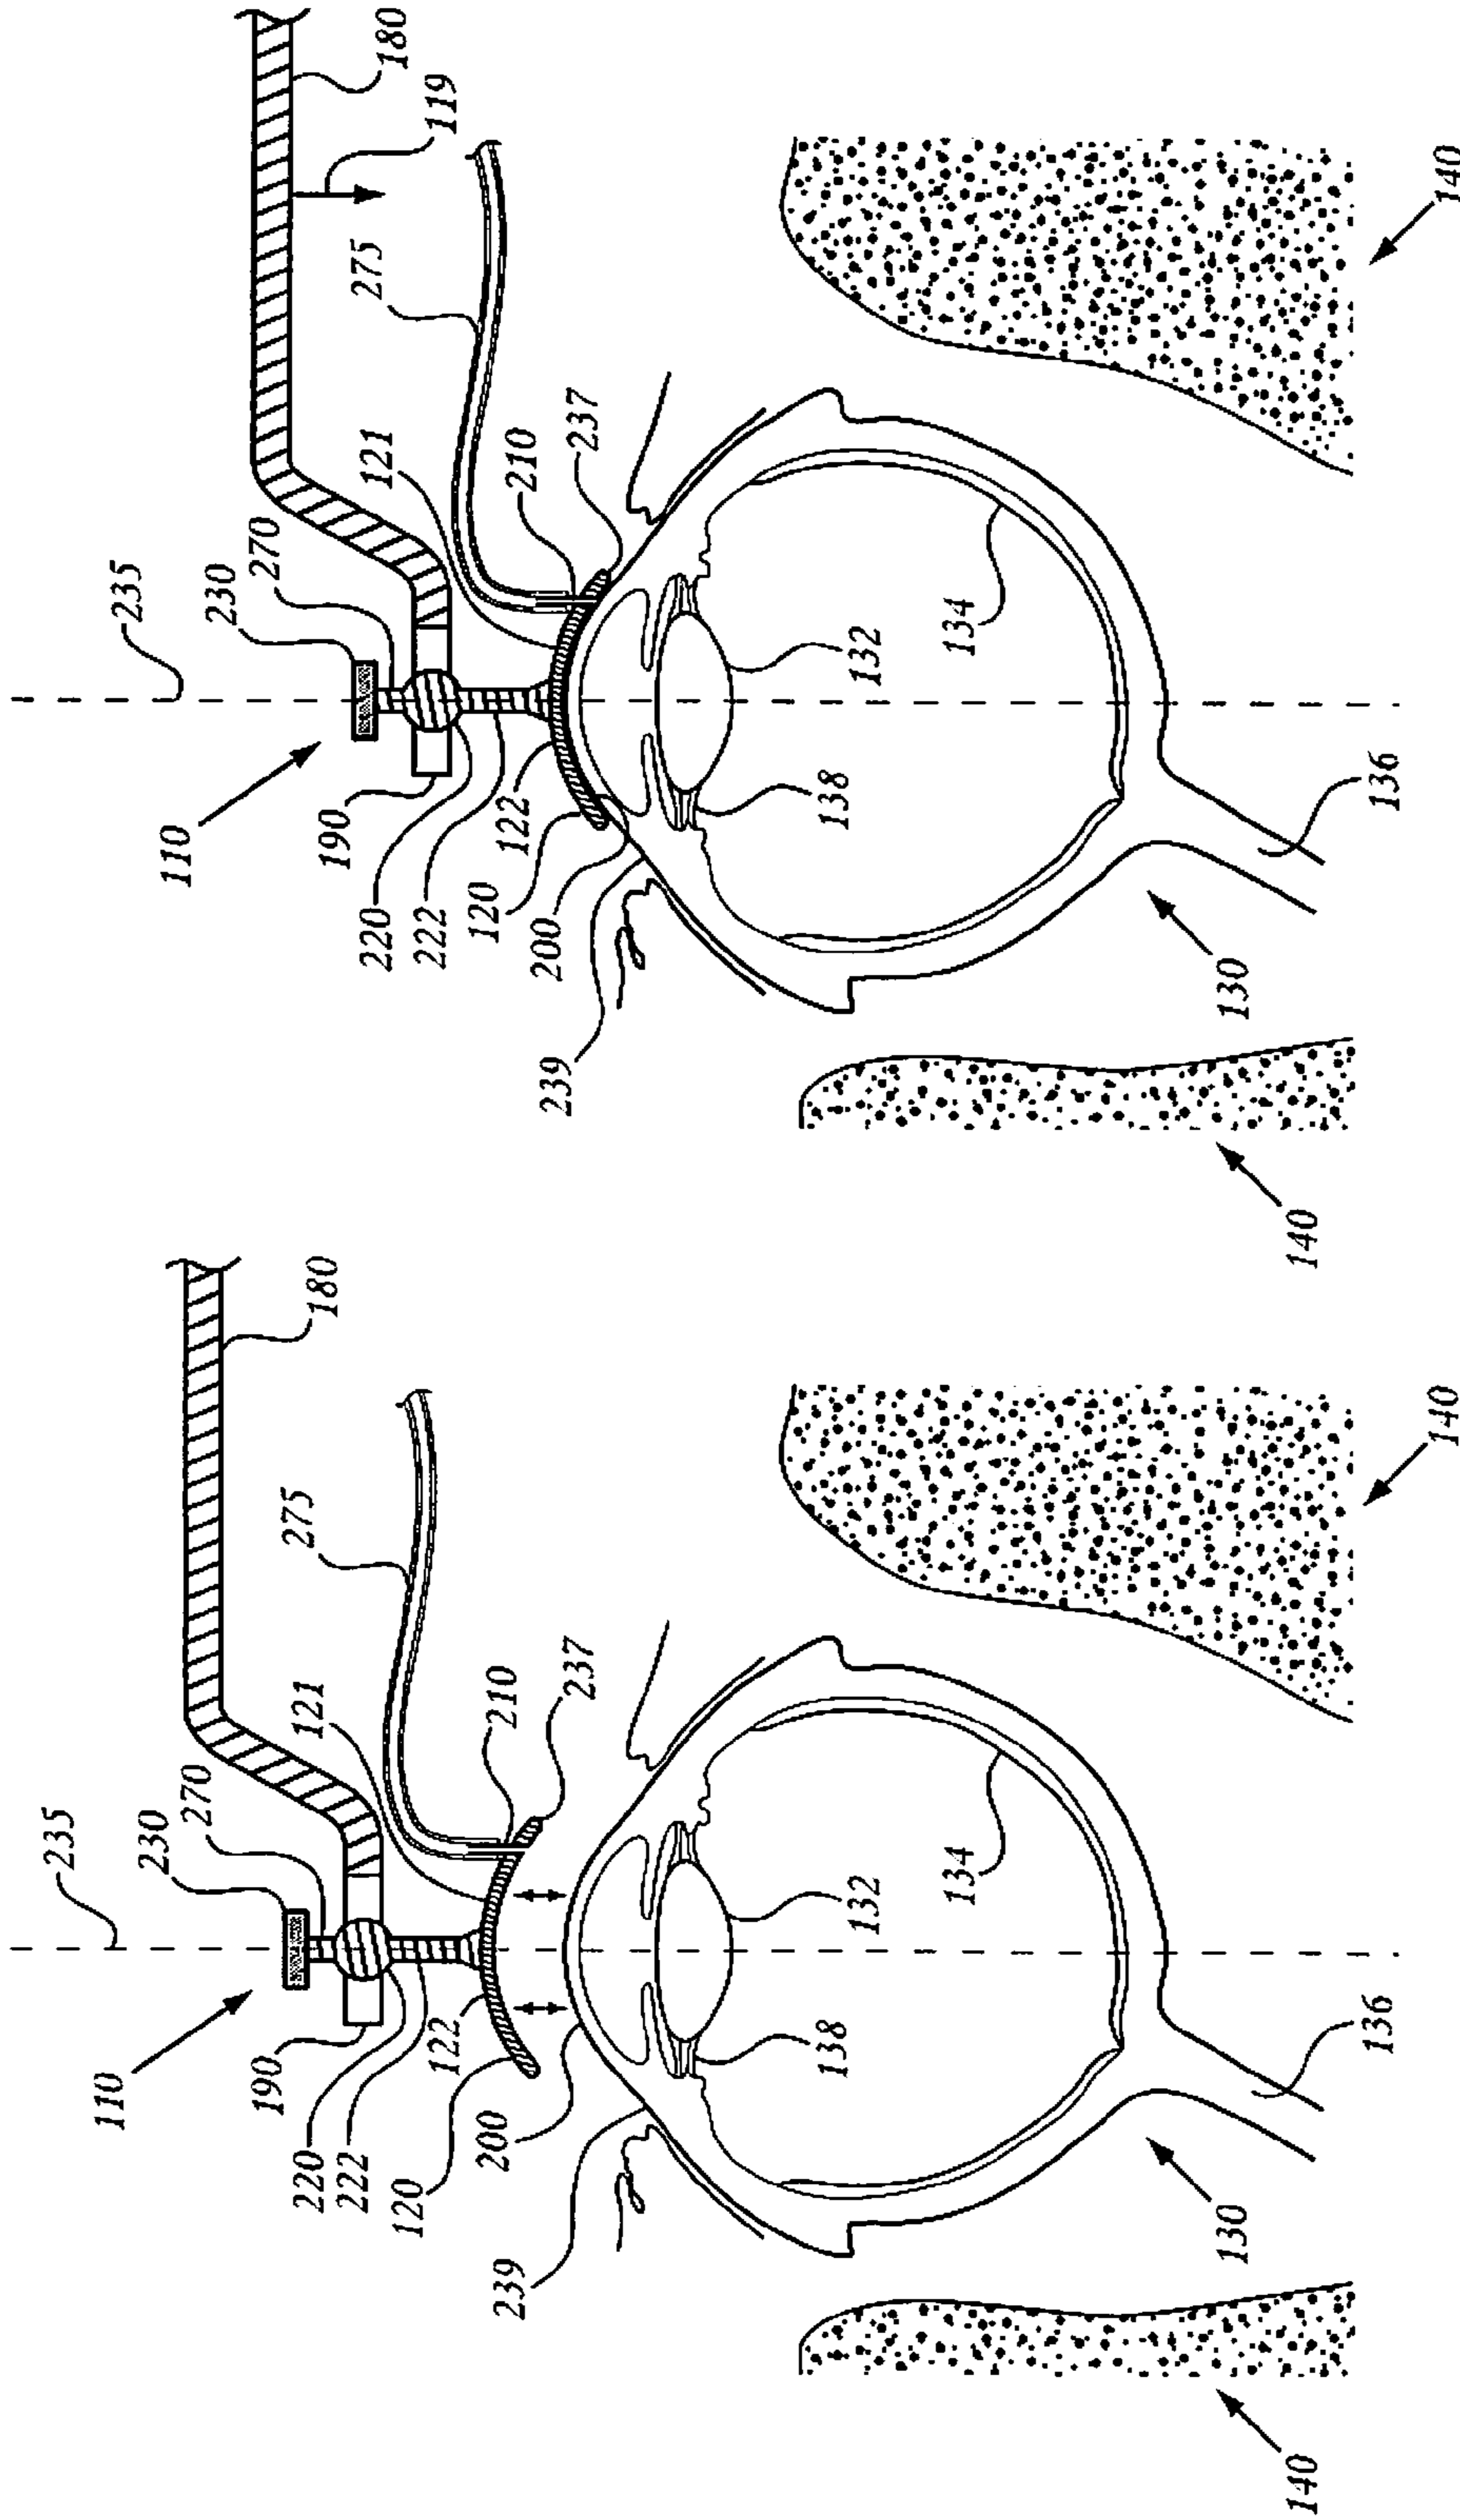


FIG. 2B

FIG. 2A

FIG. 3A

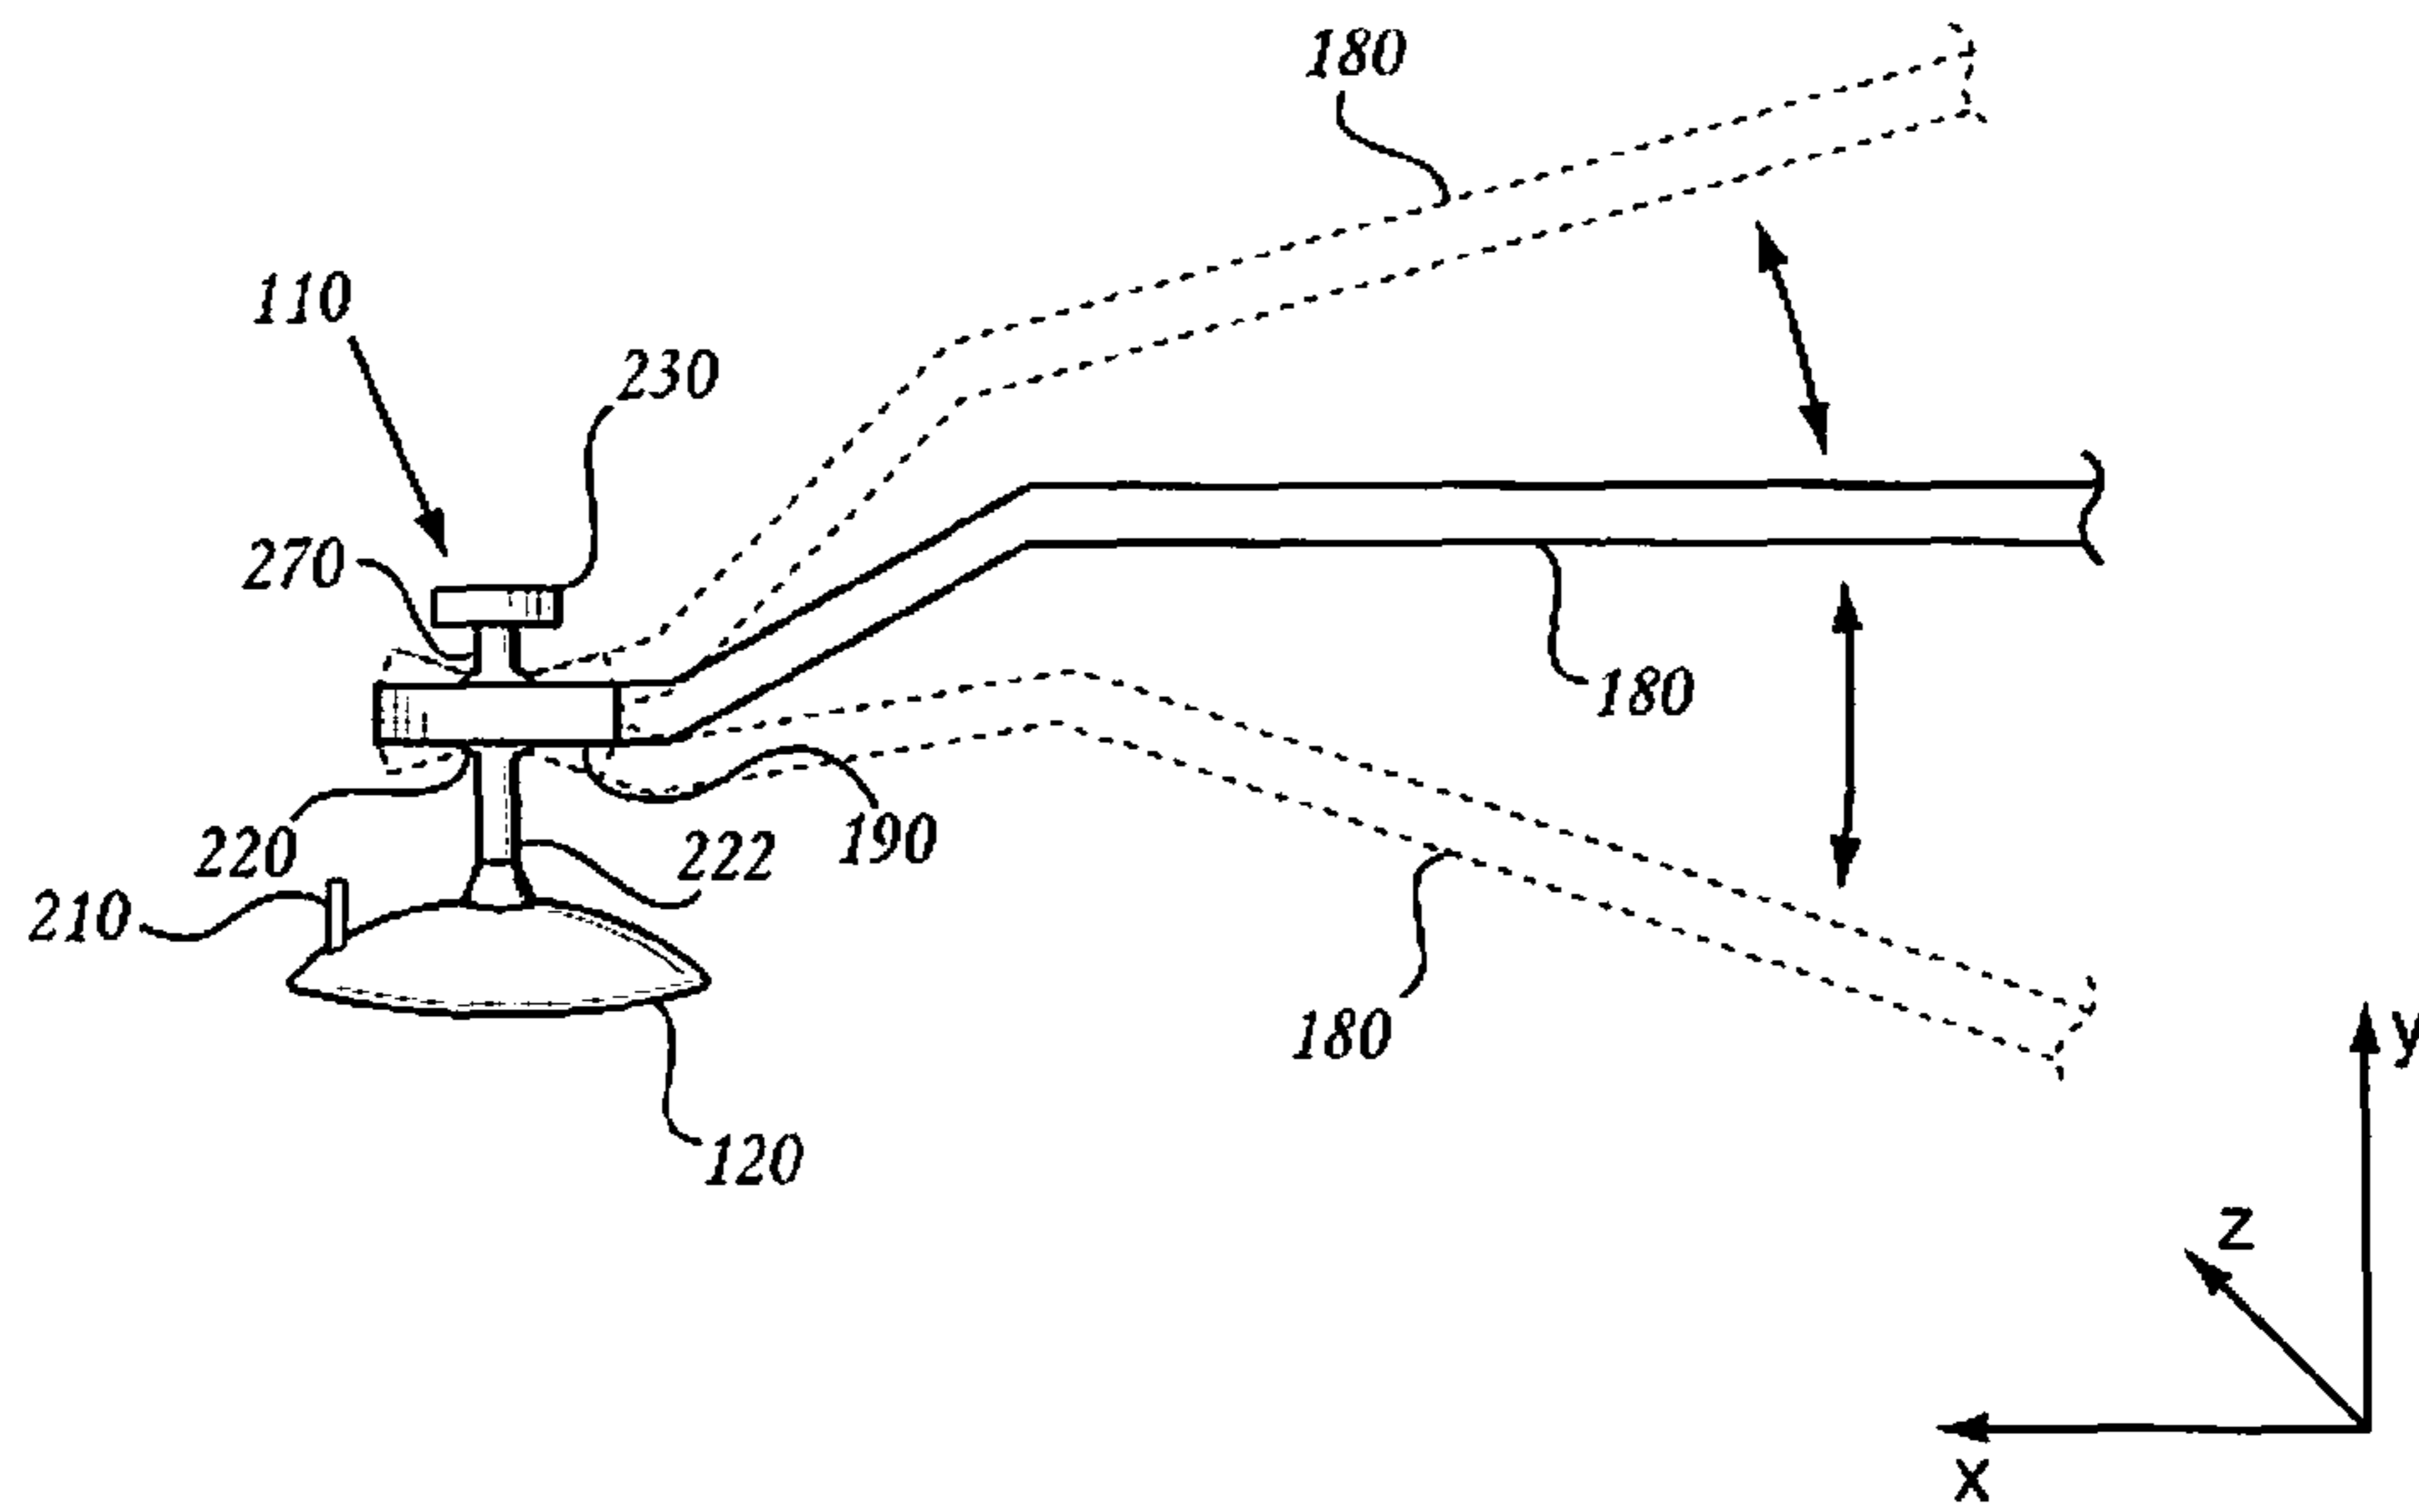


FIG. 3B

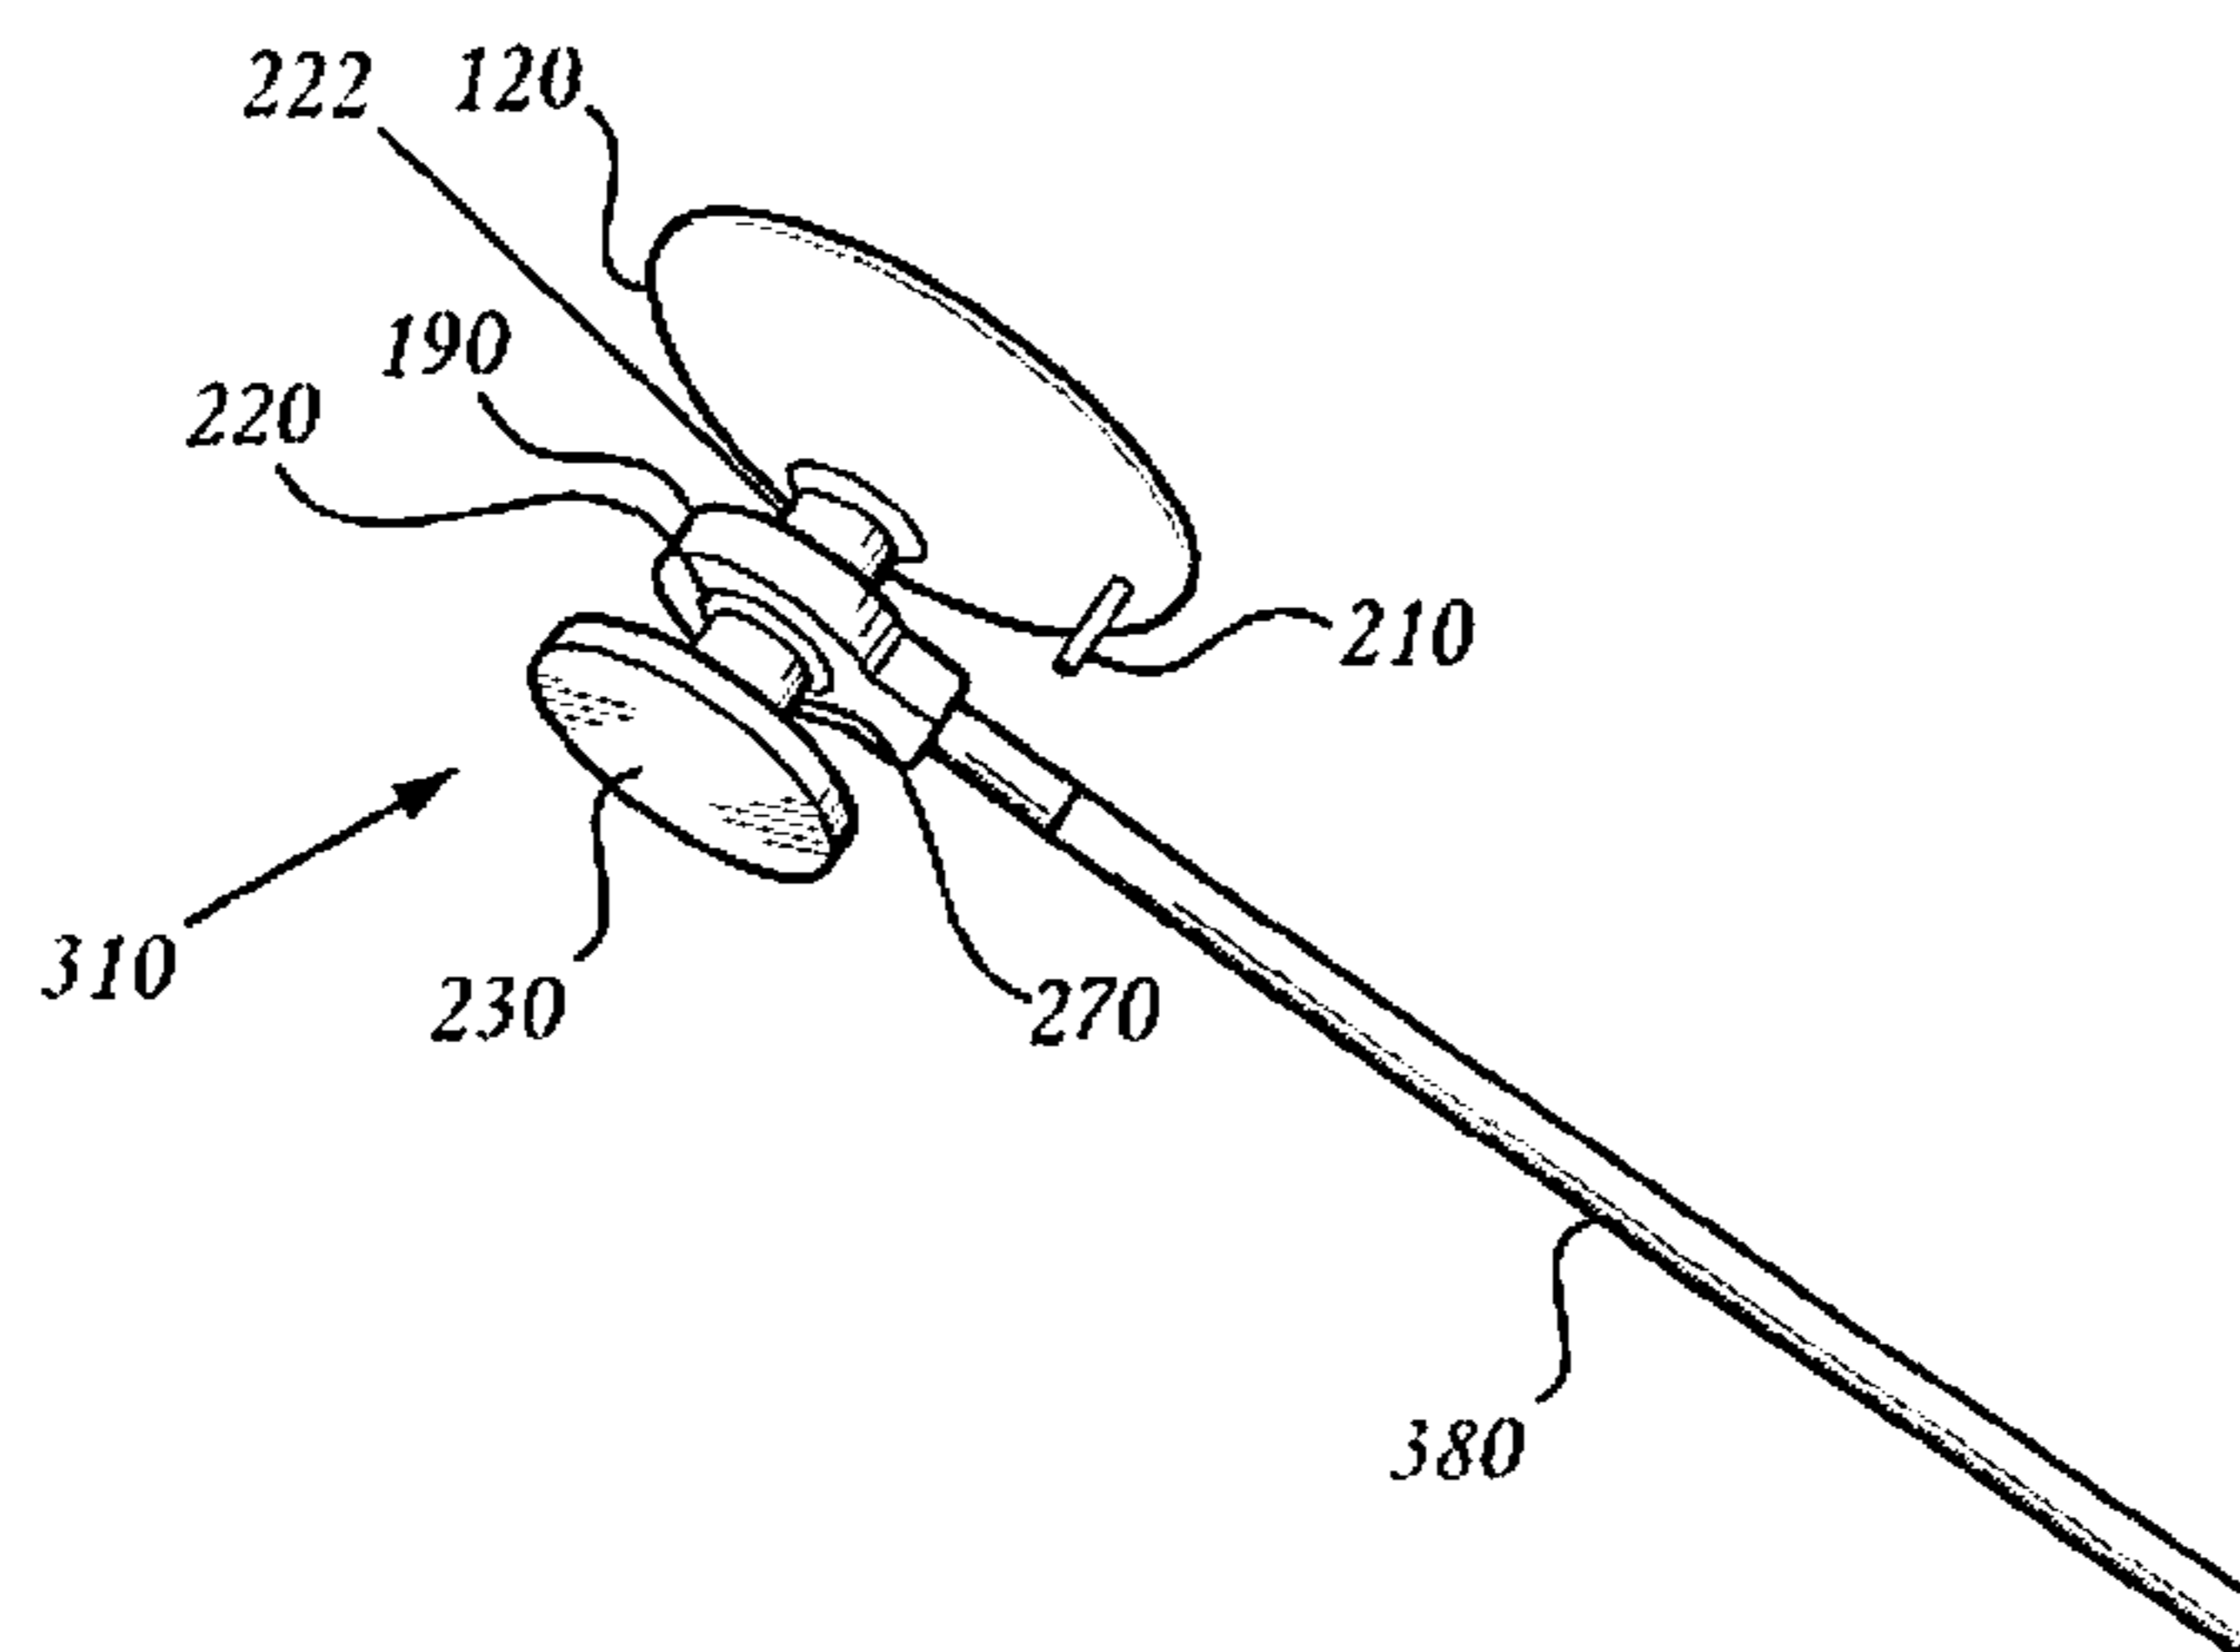


FIG. 3C

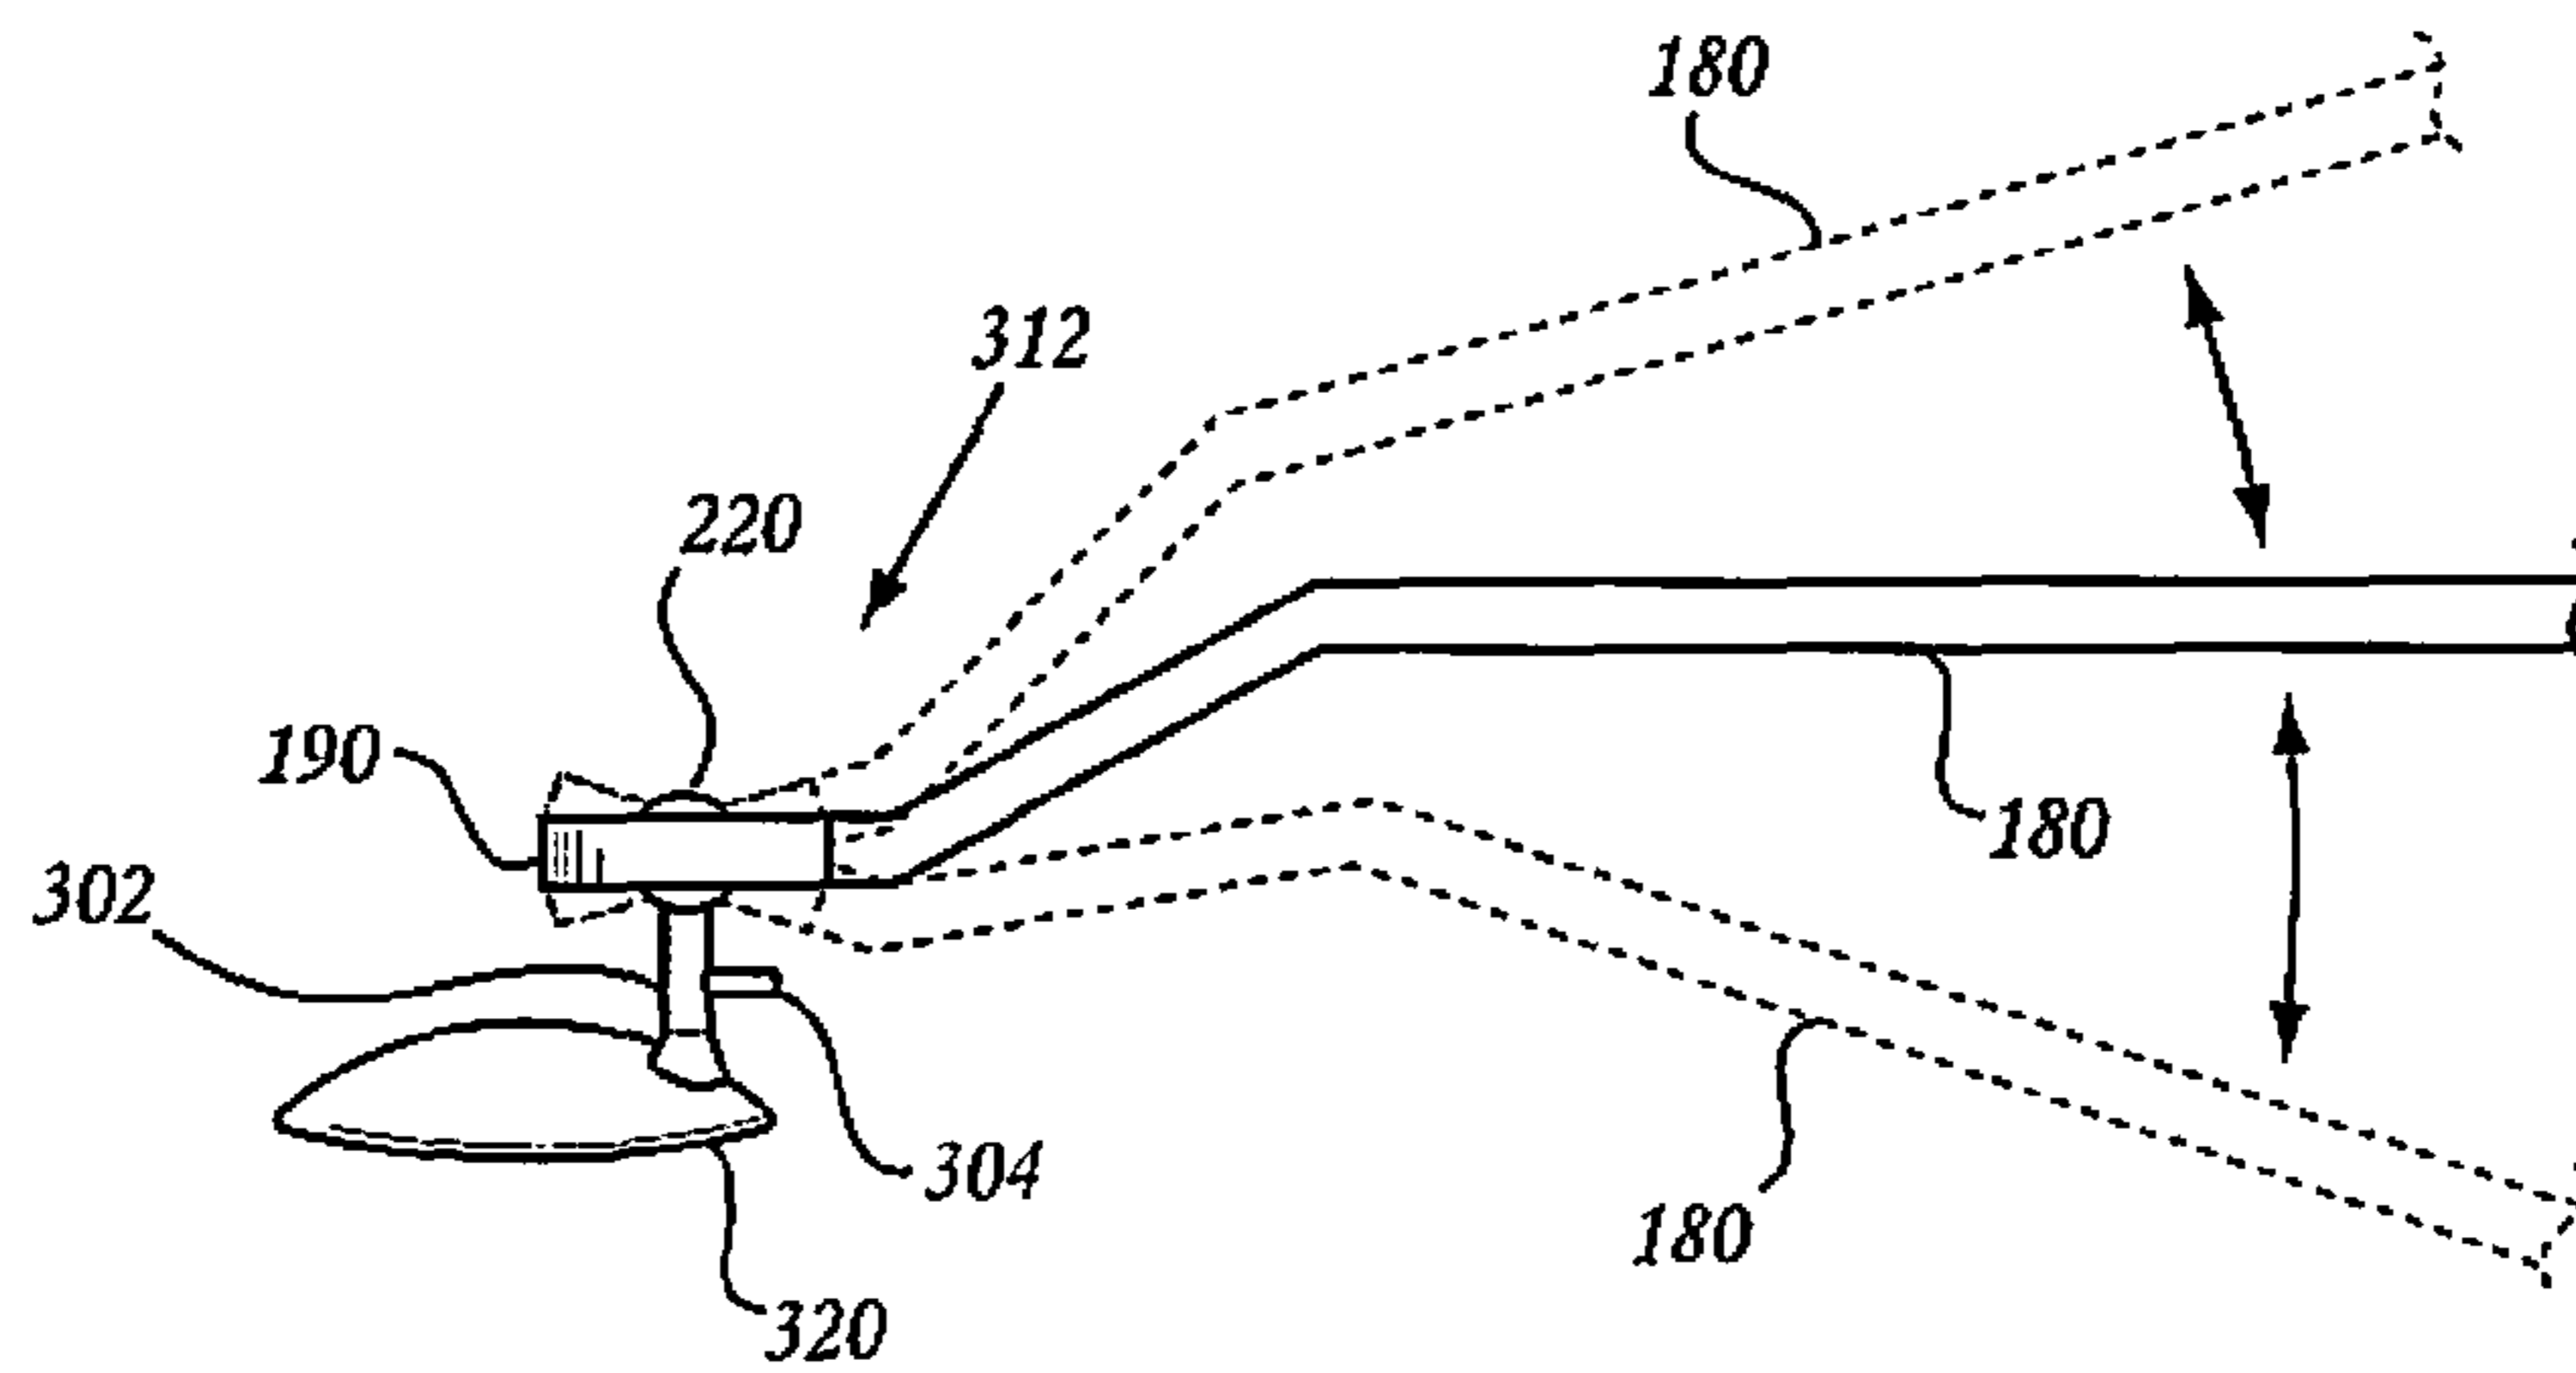
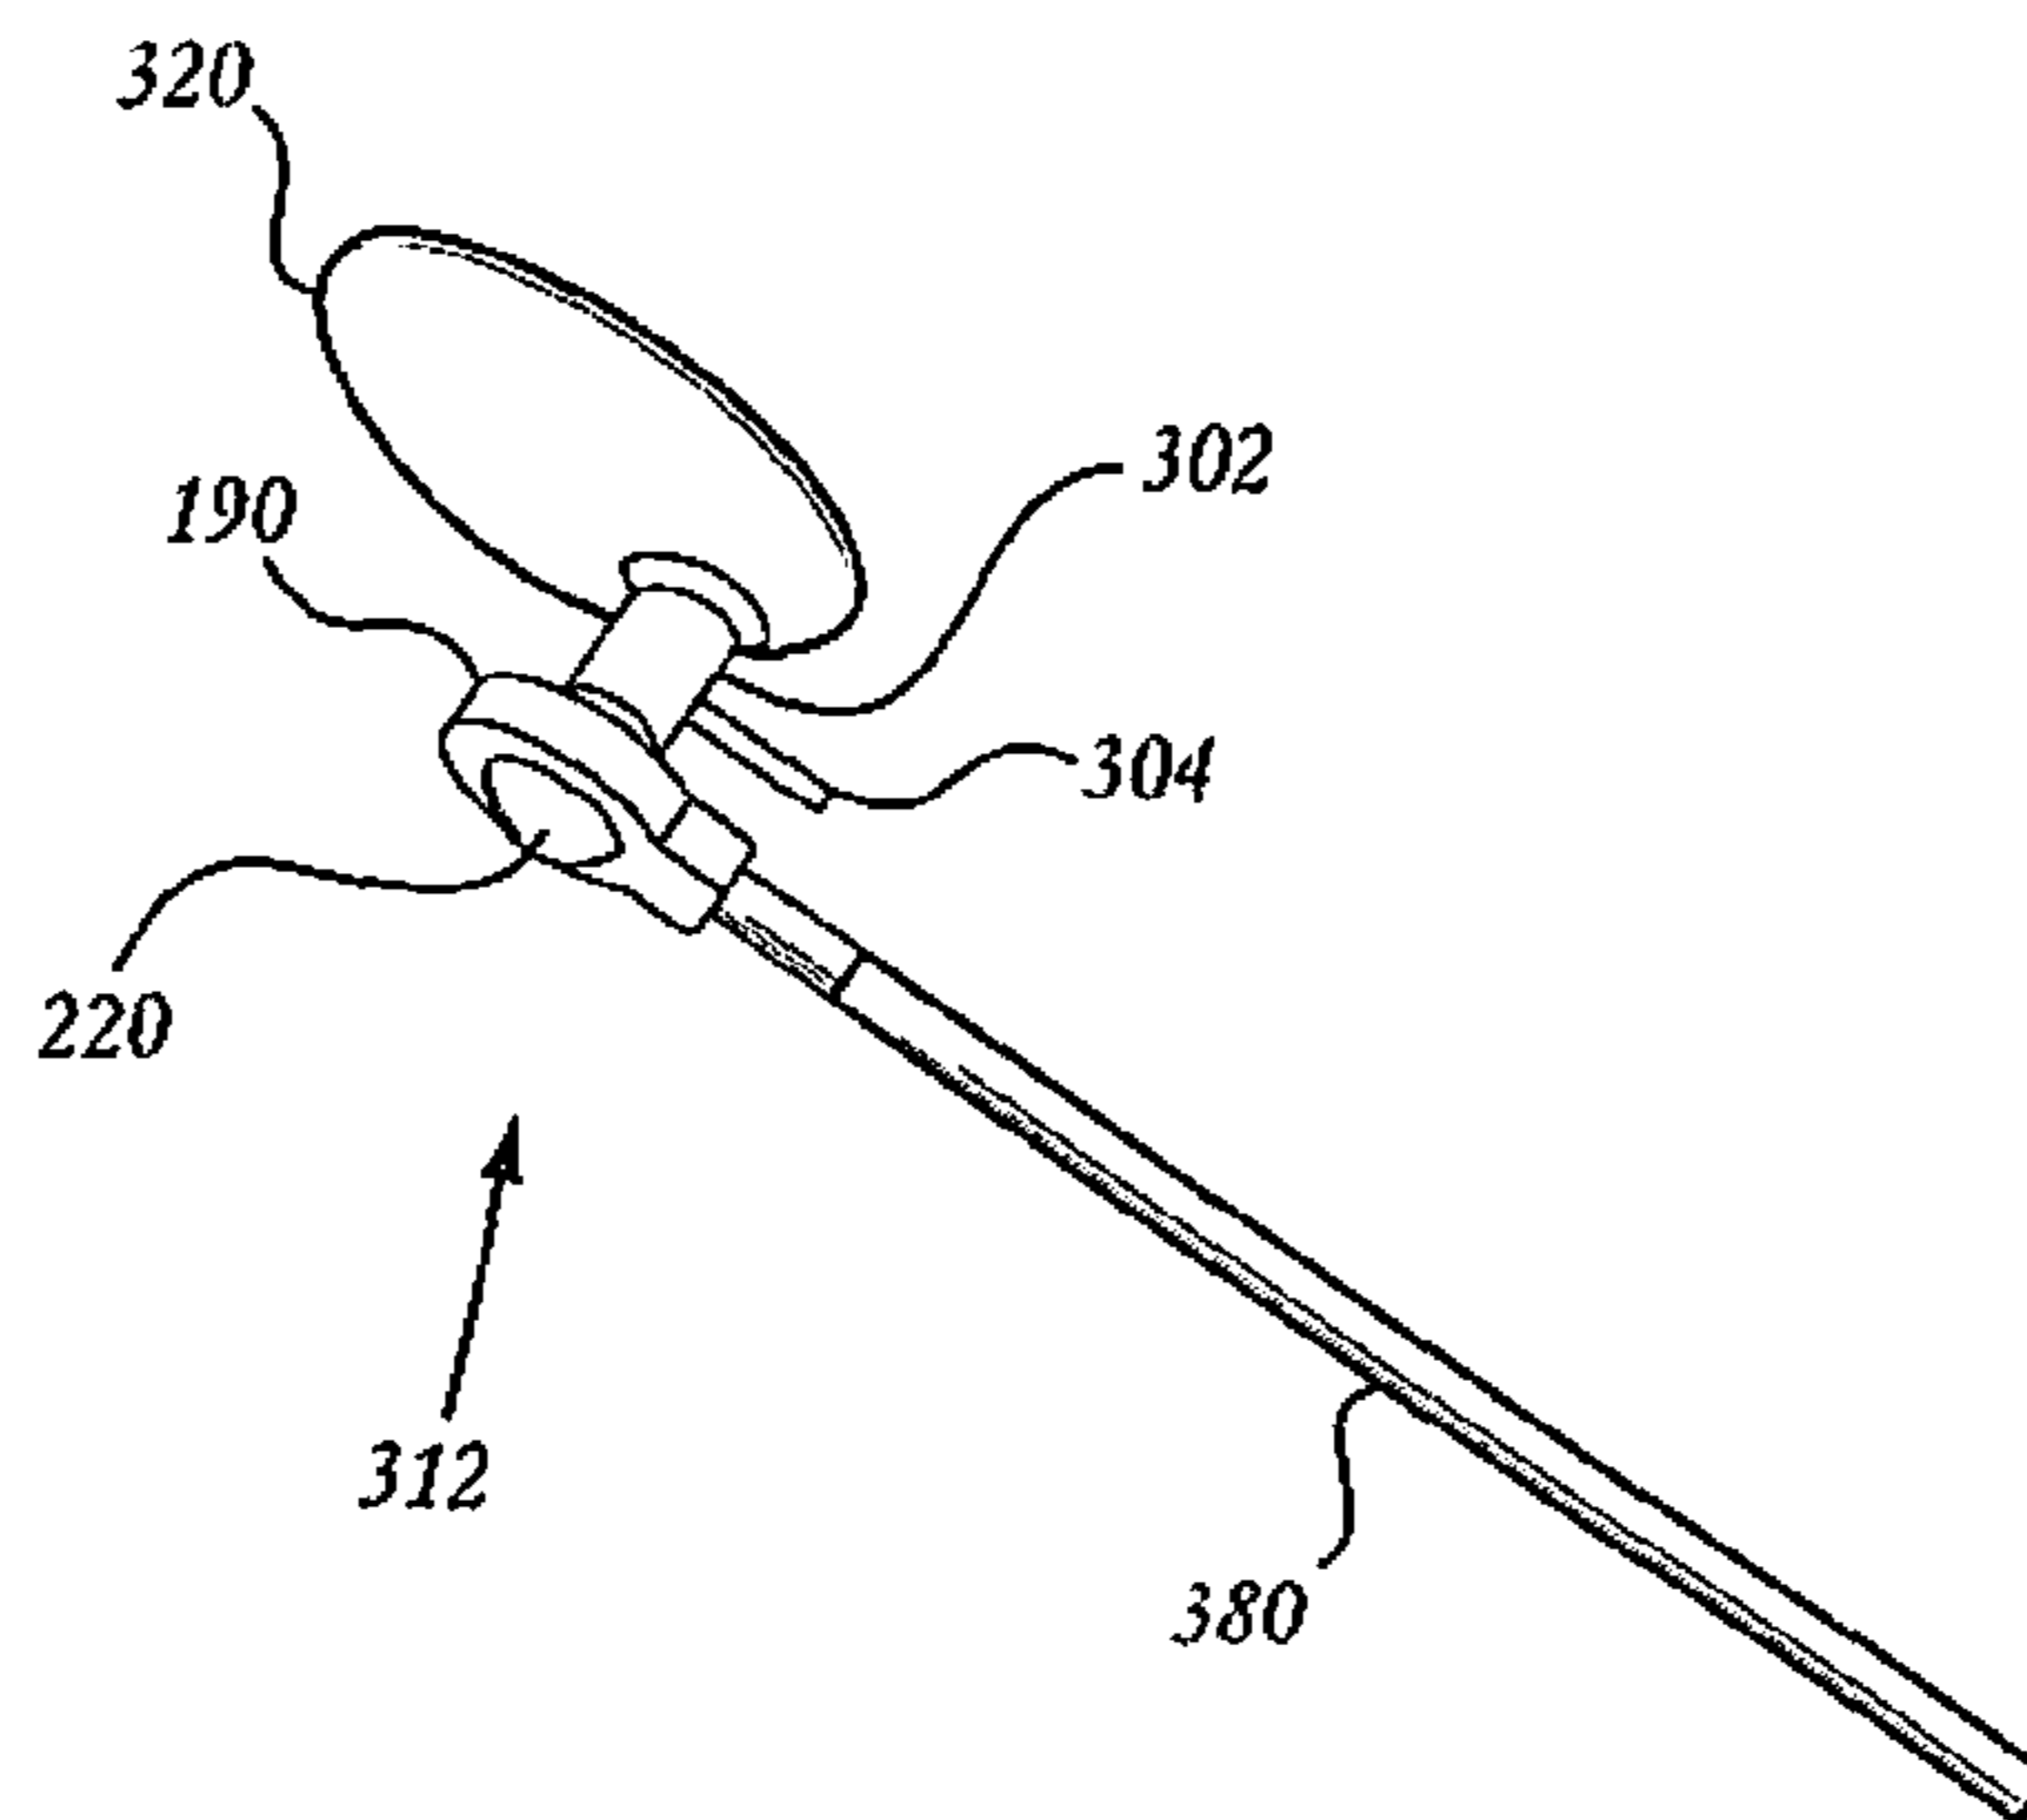


FIG. 3D



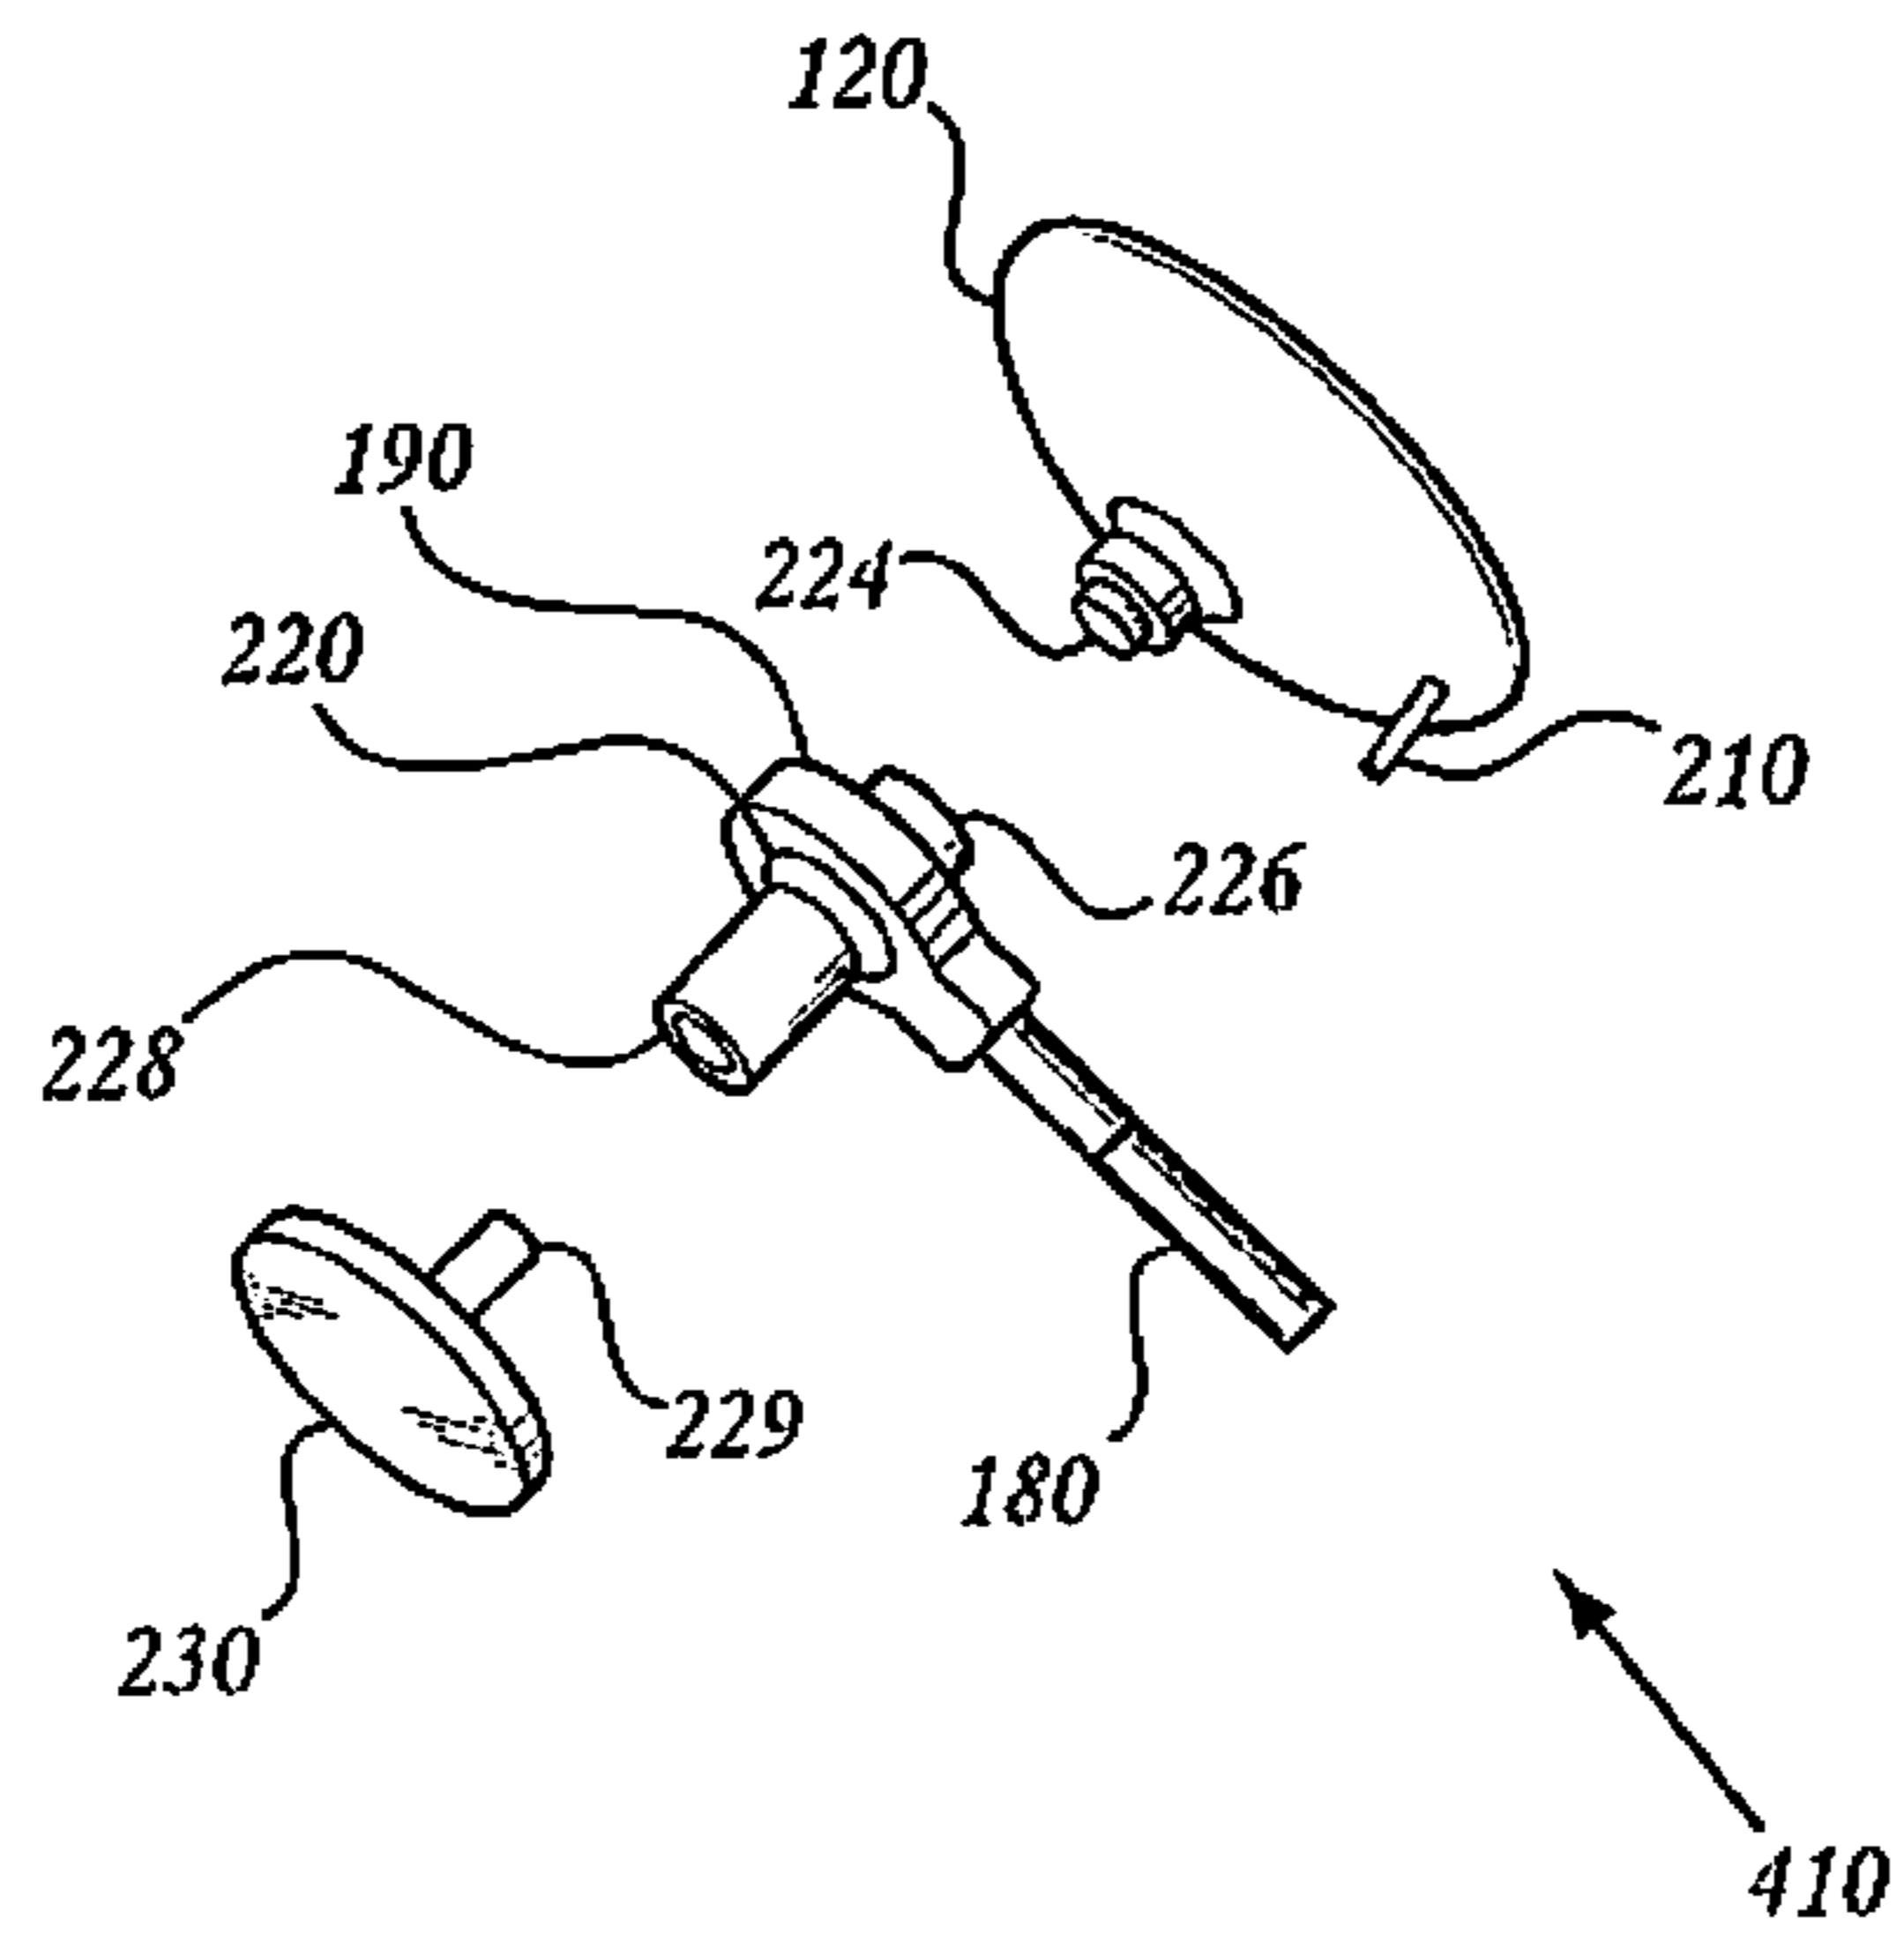


FIG. 4A



FIG. 4B

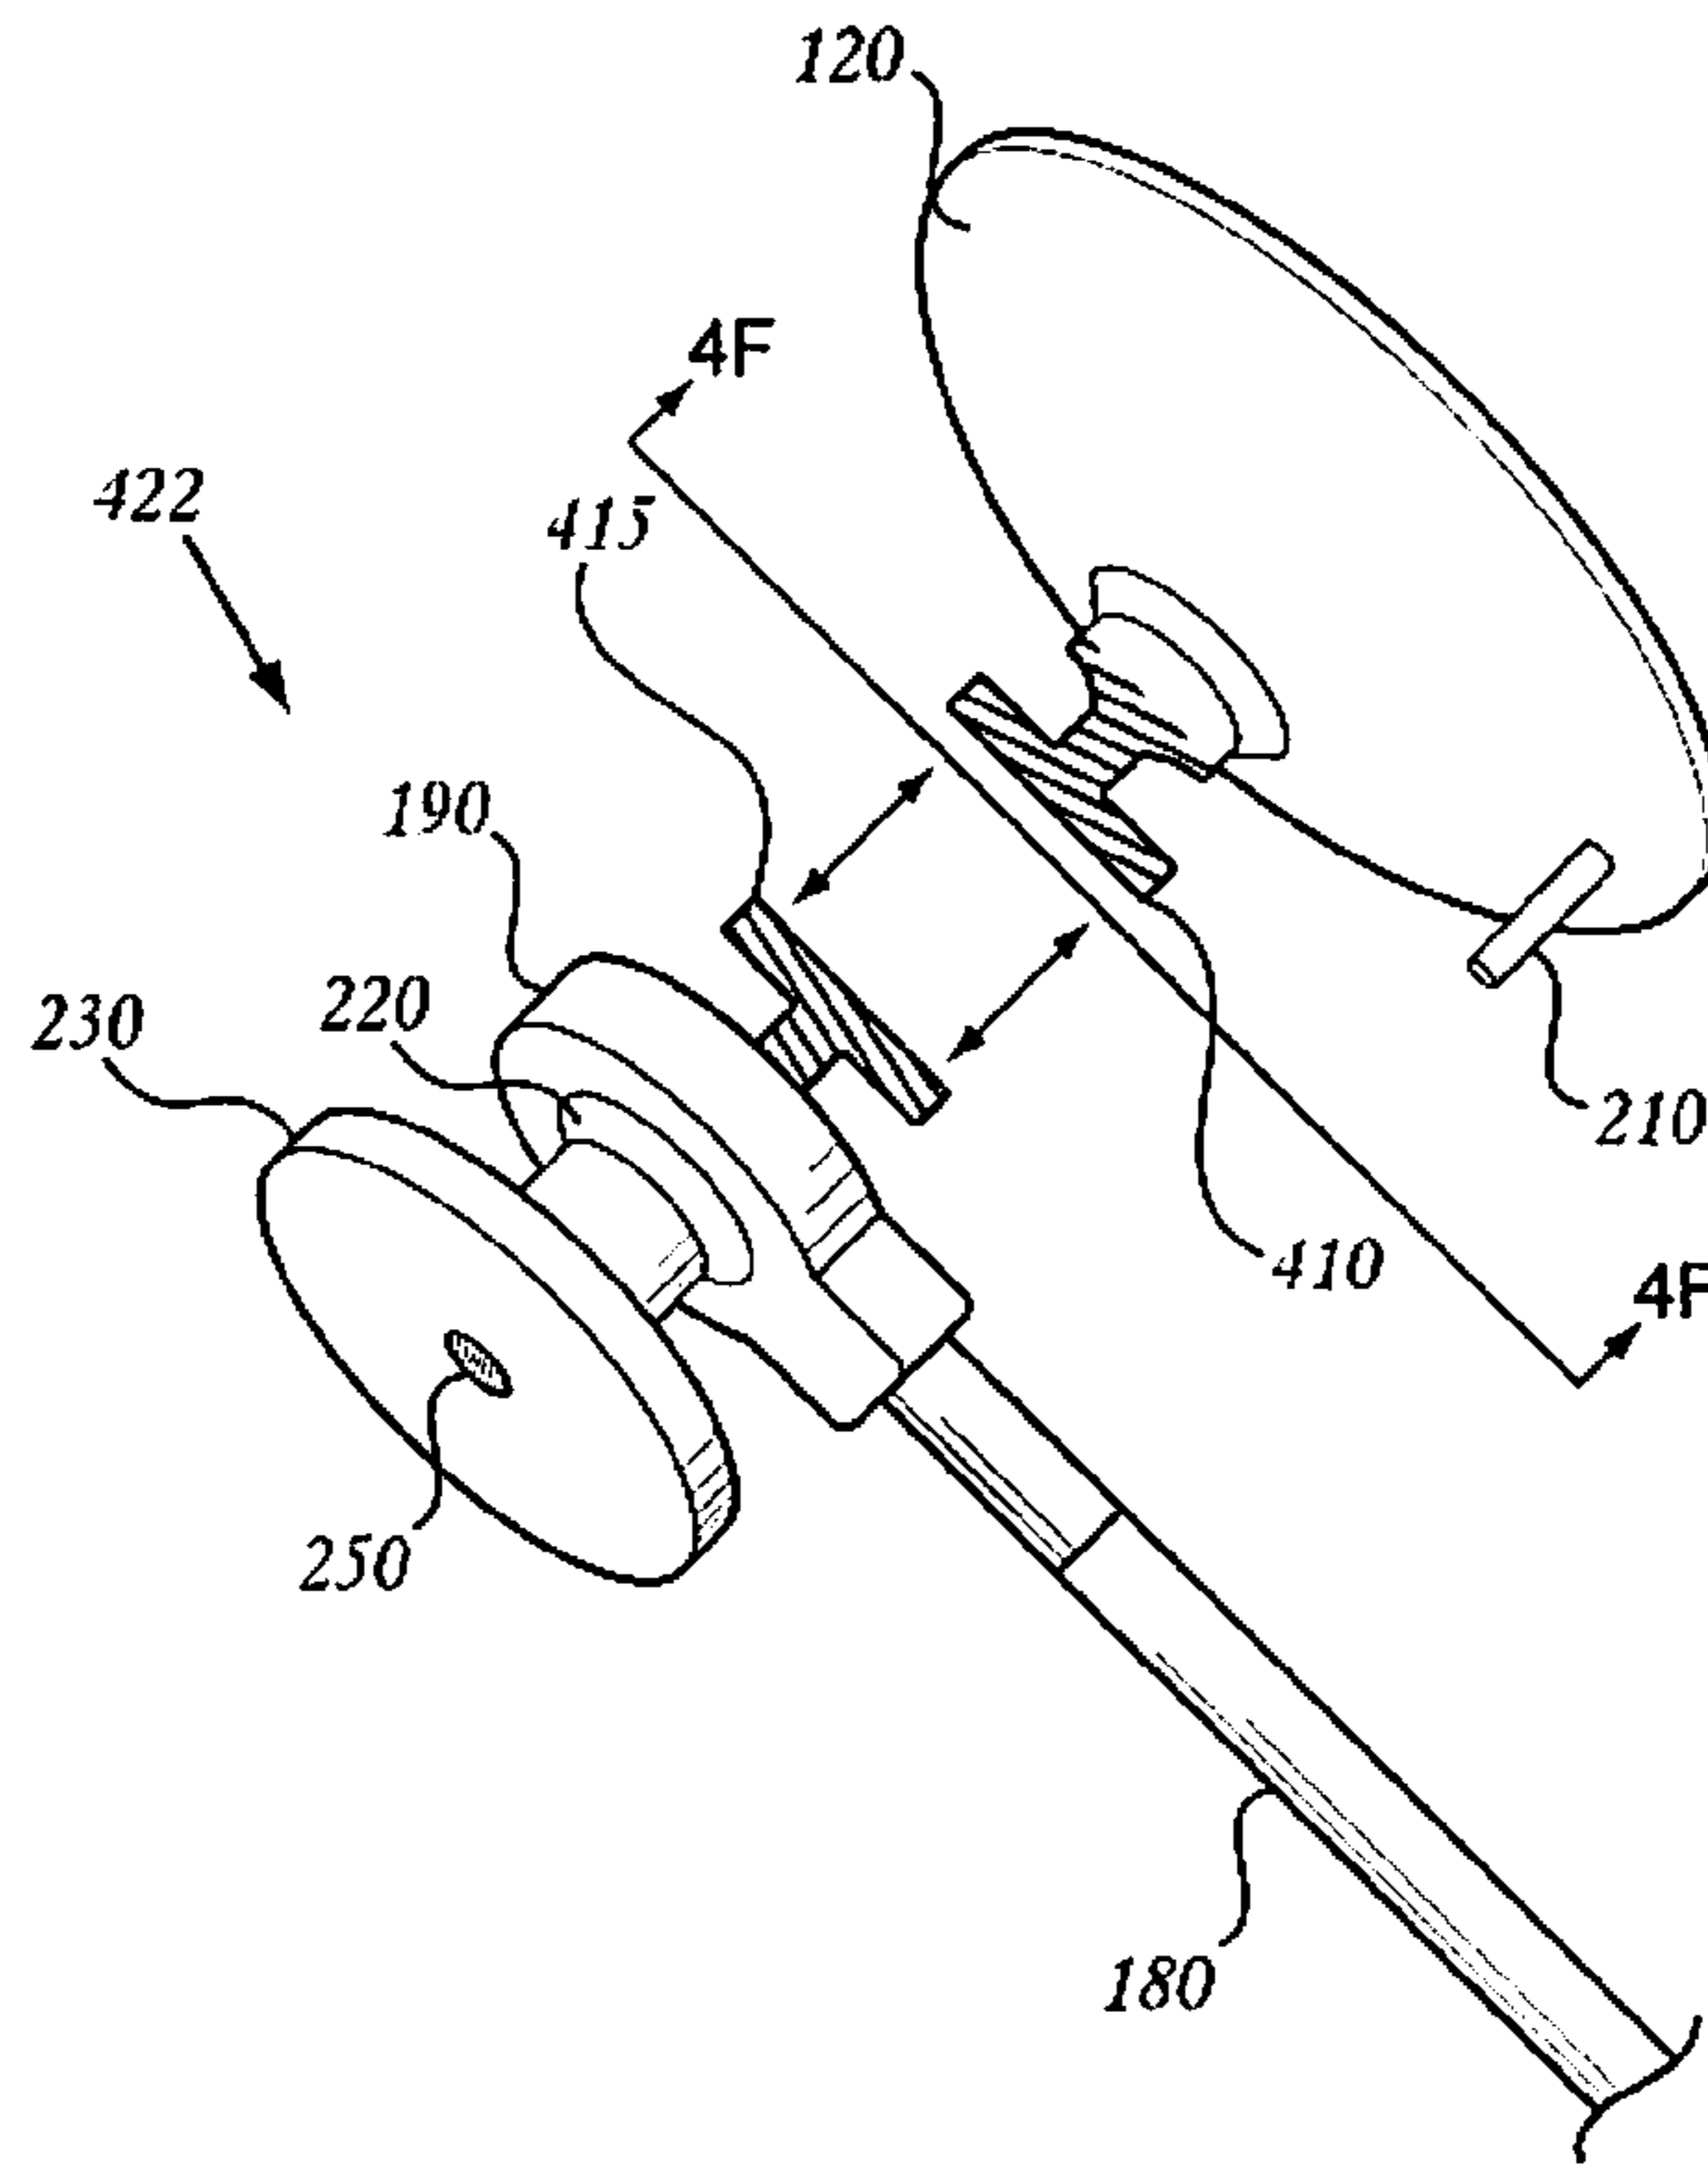


FIG. 4C

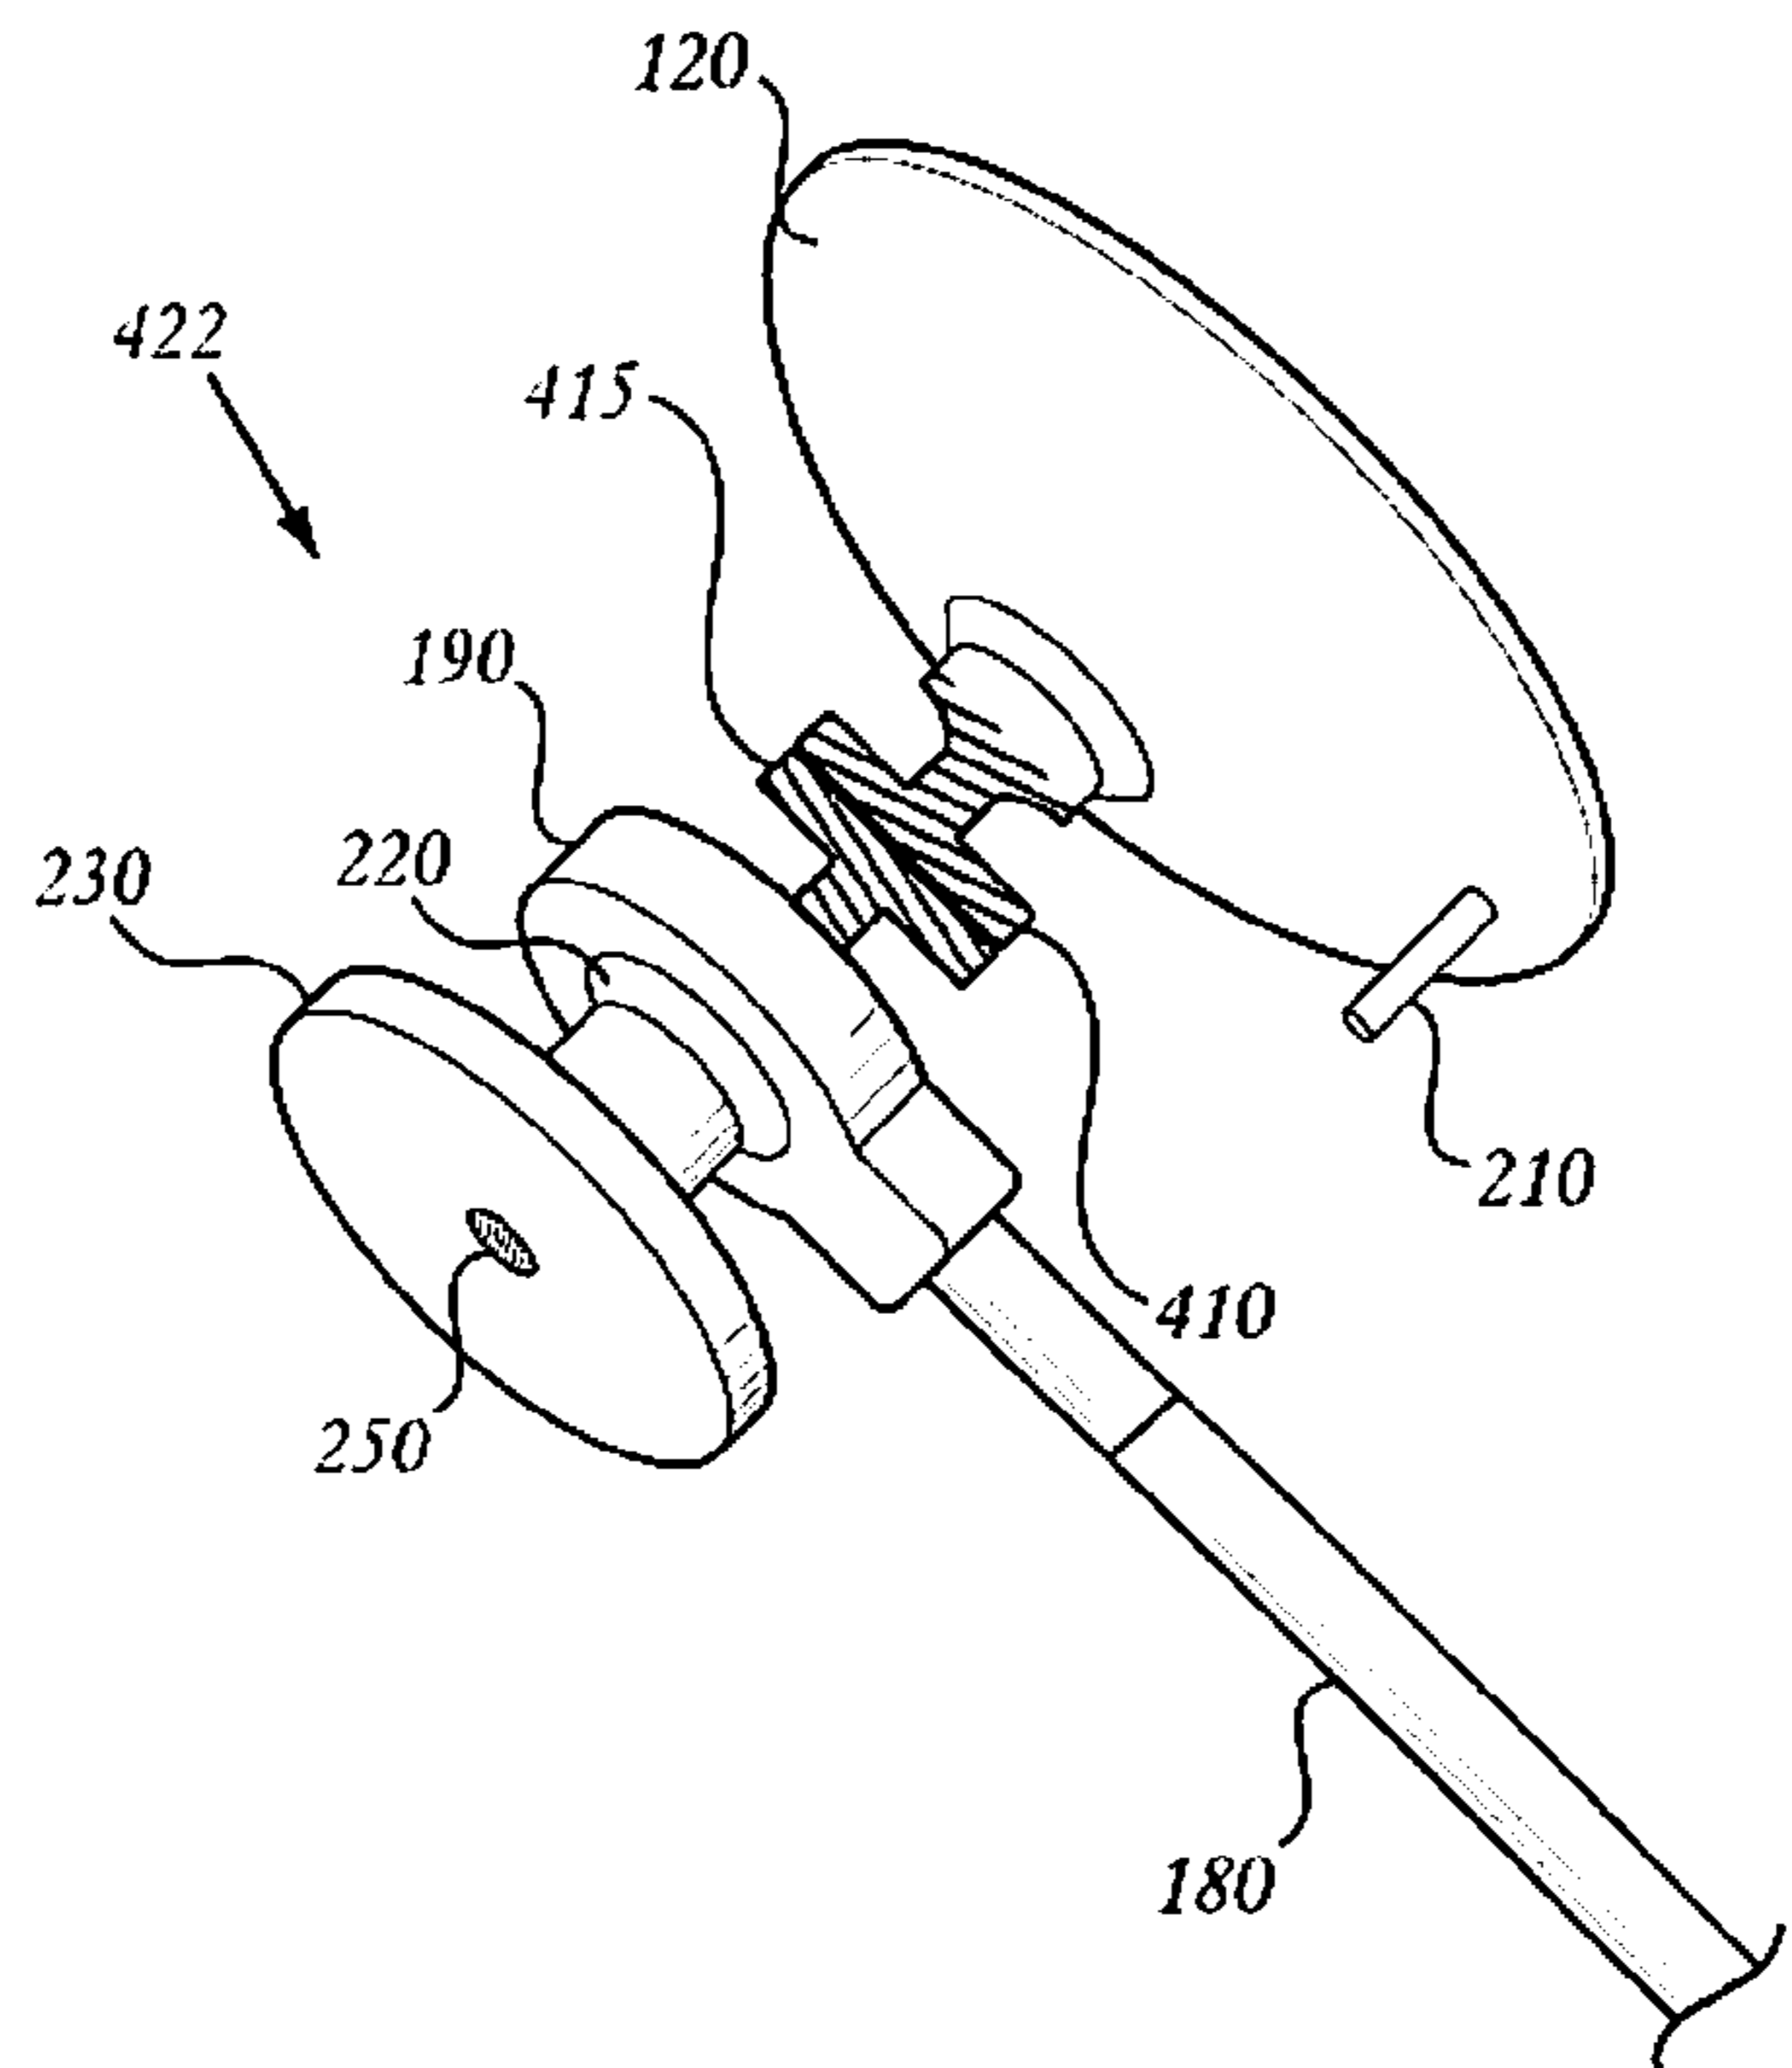


FIG. 4D

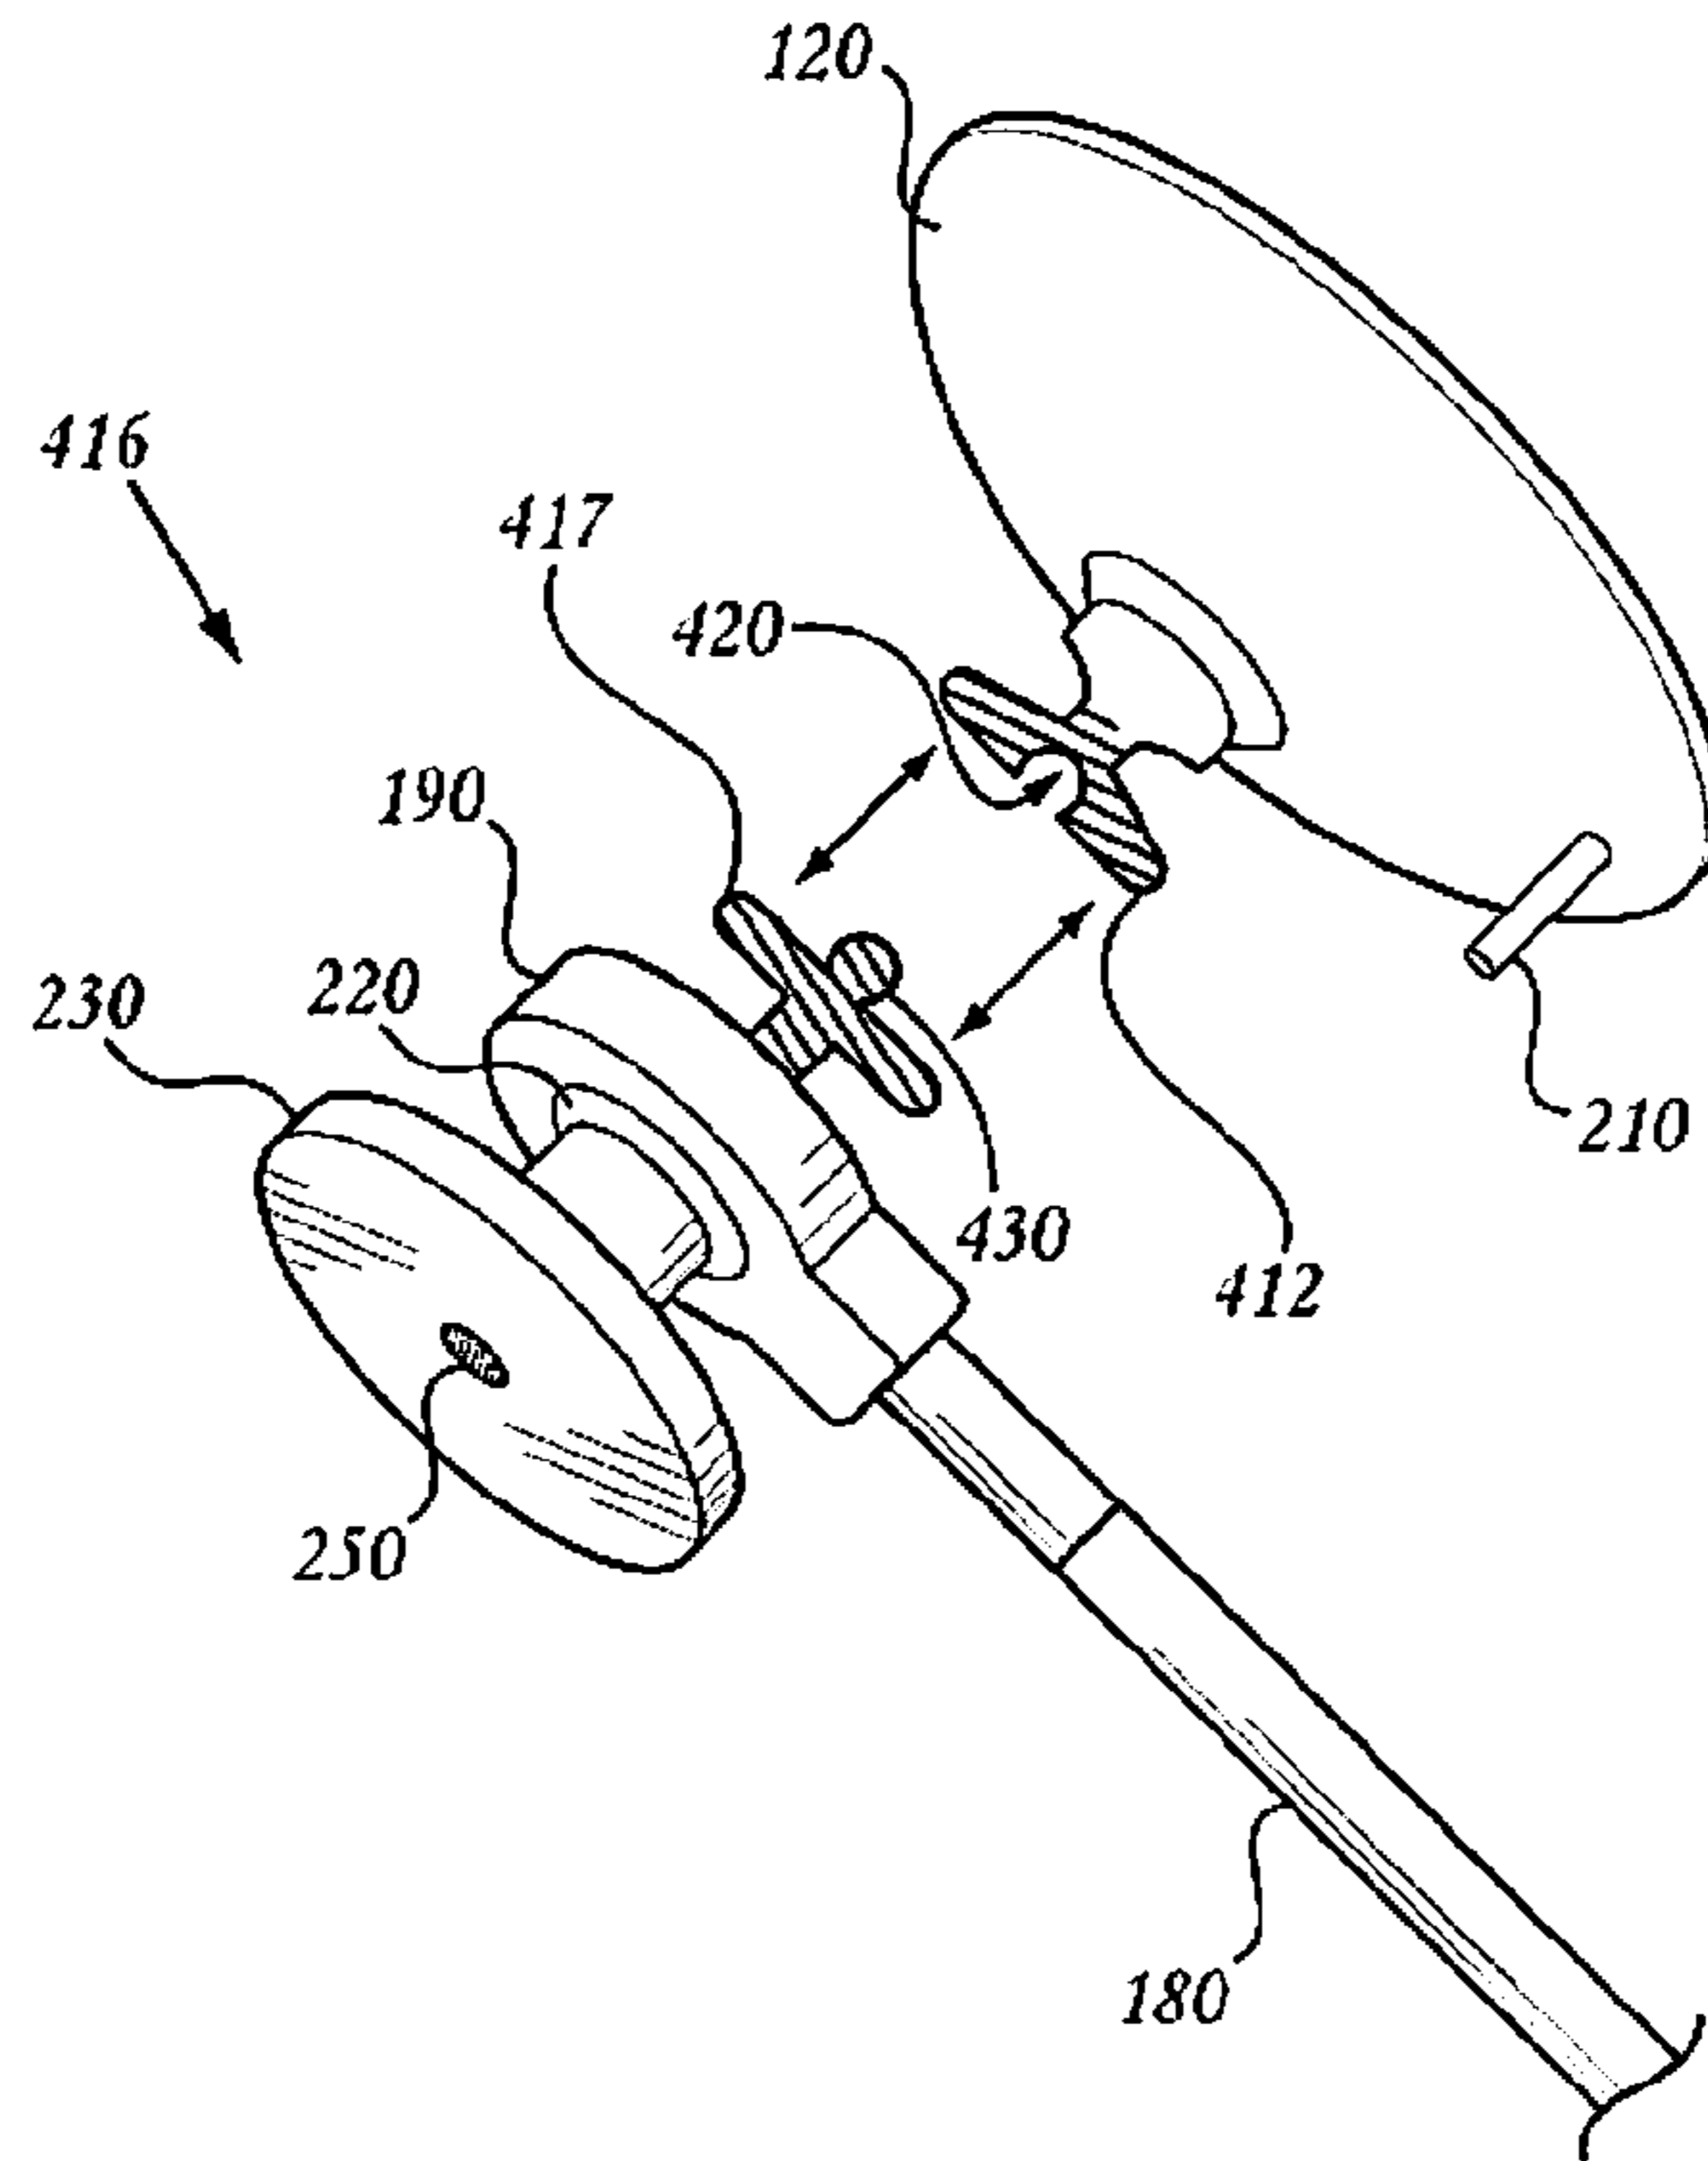
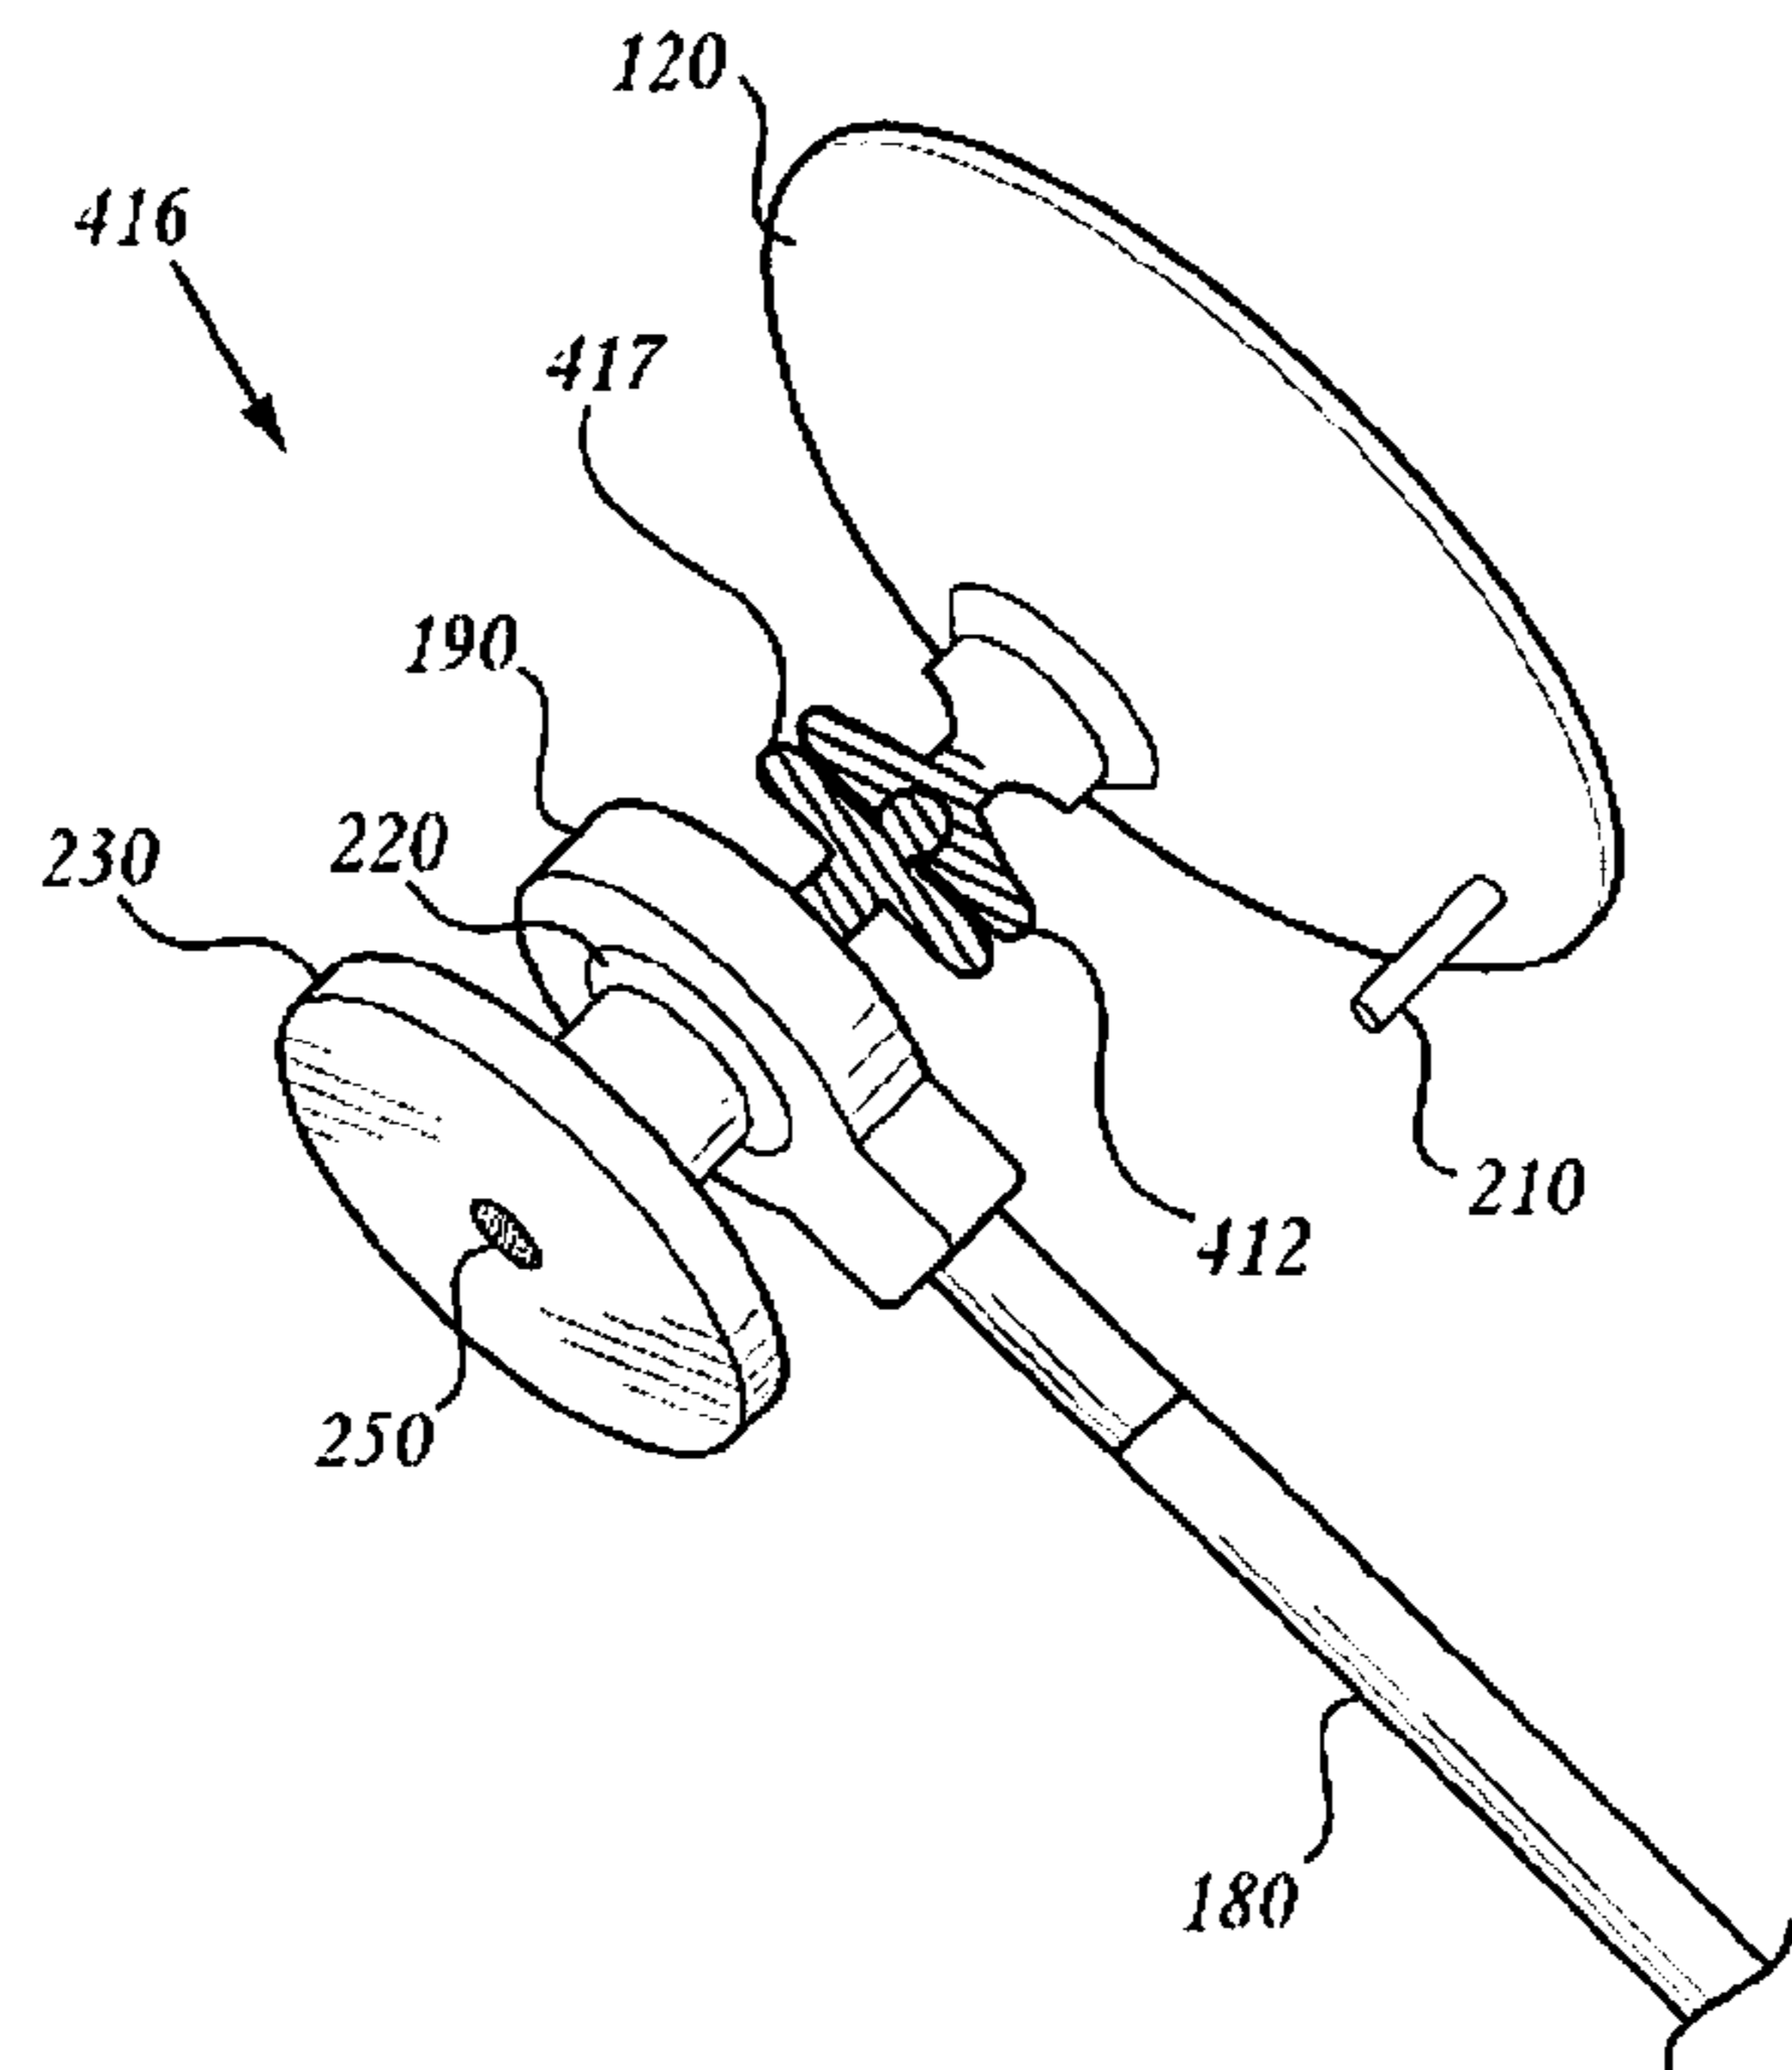


FIG. 4E



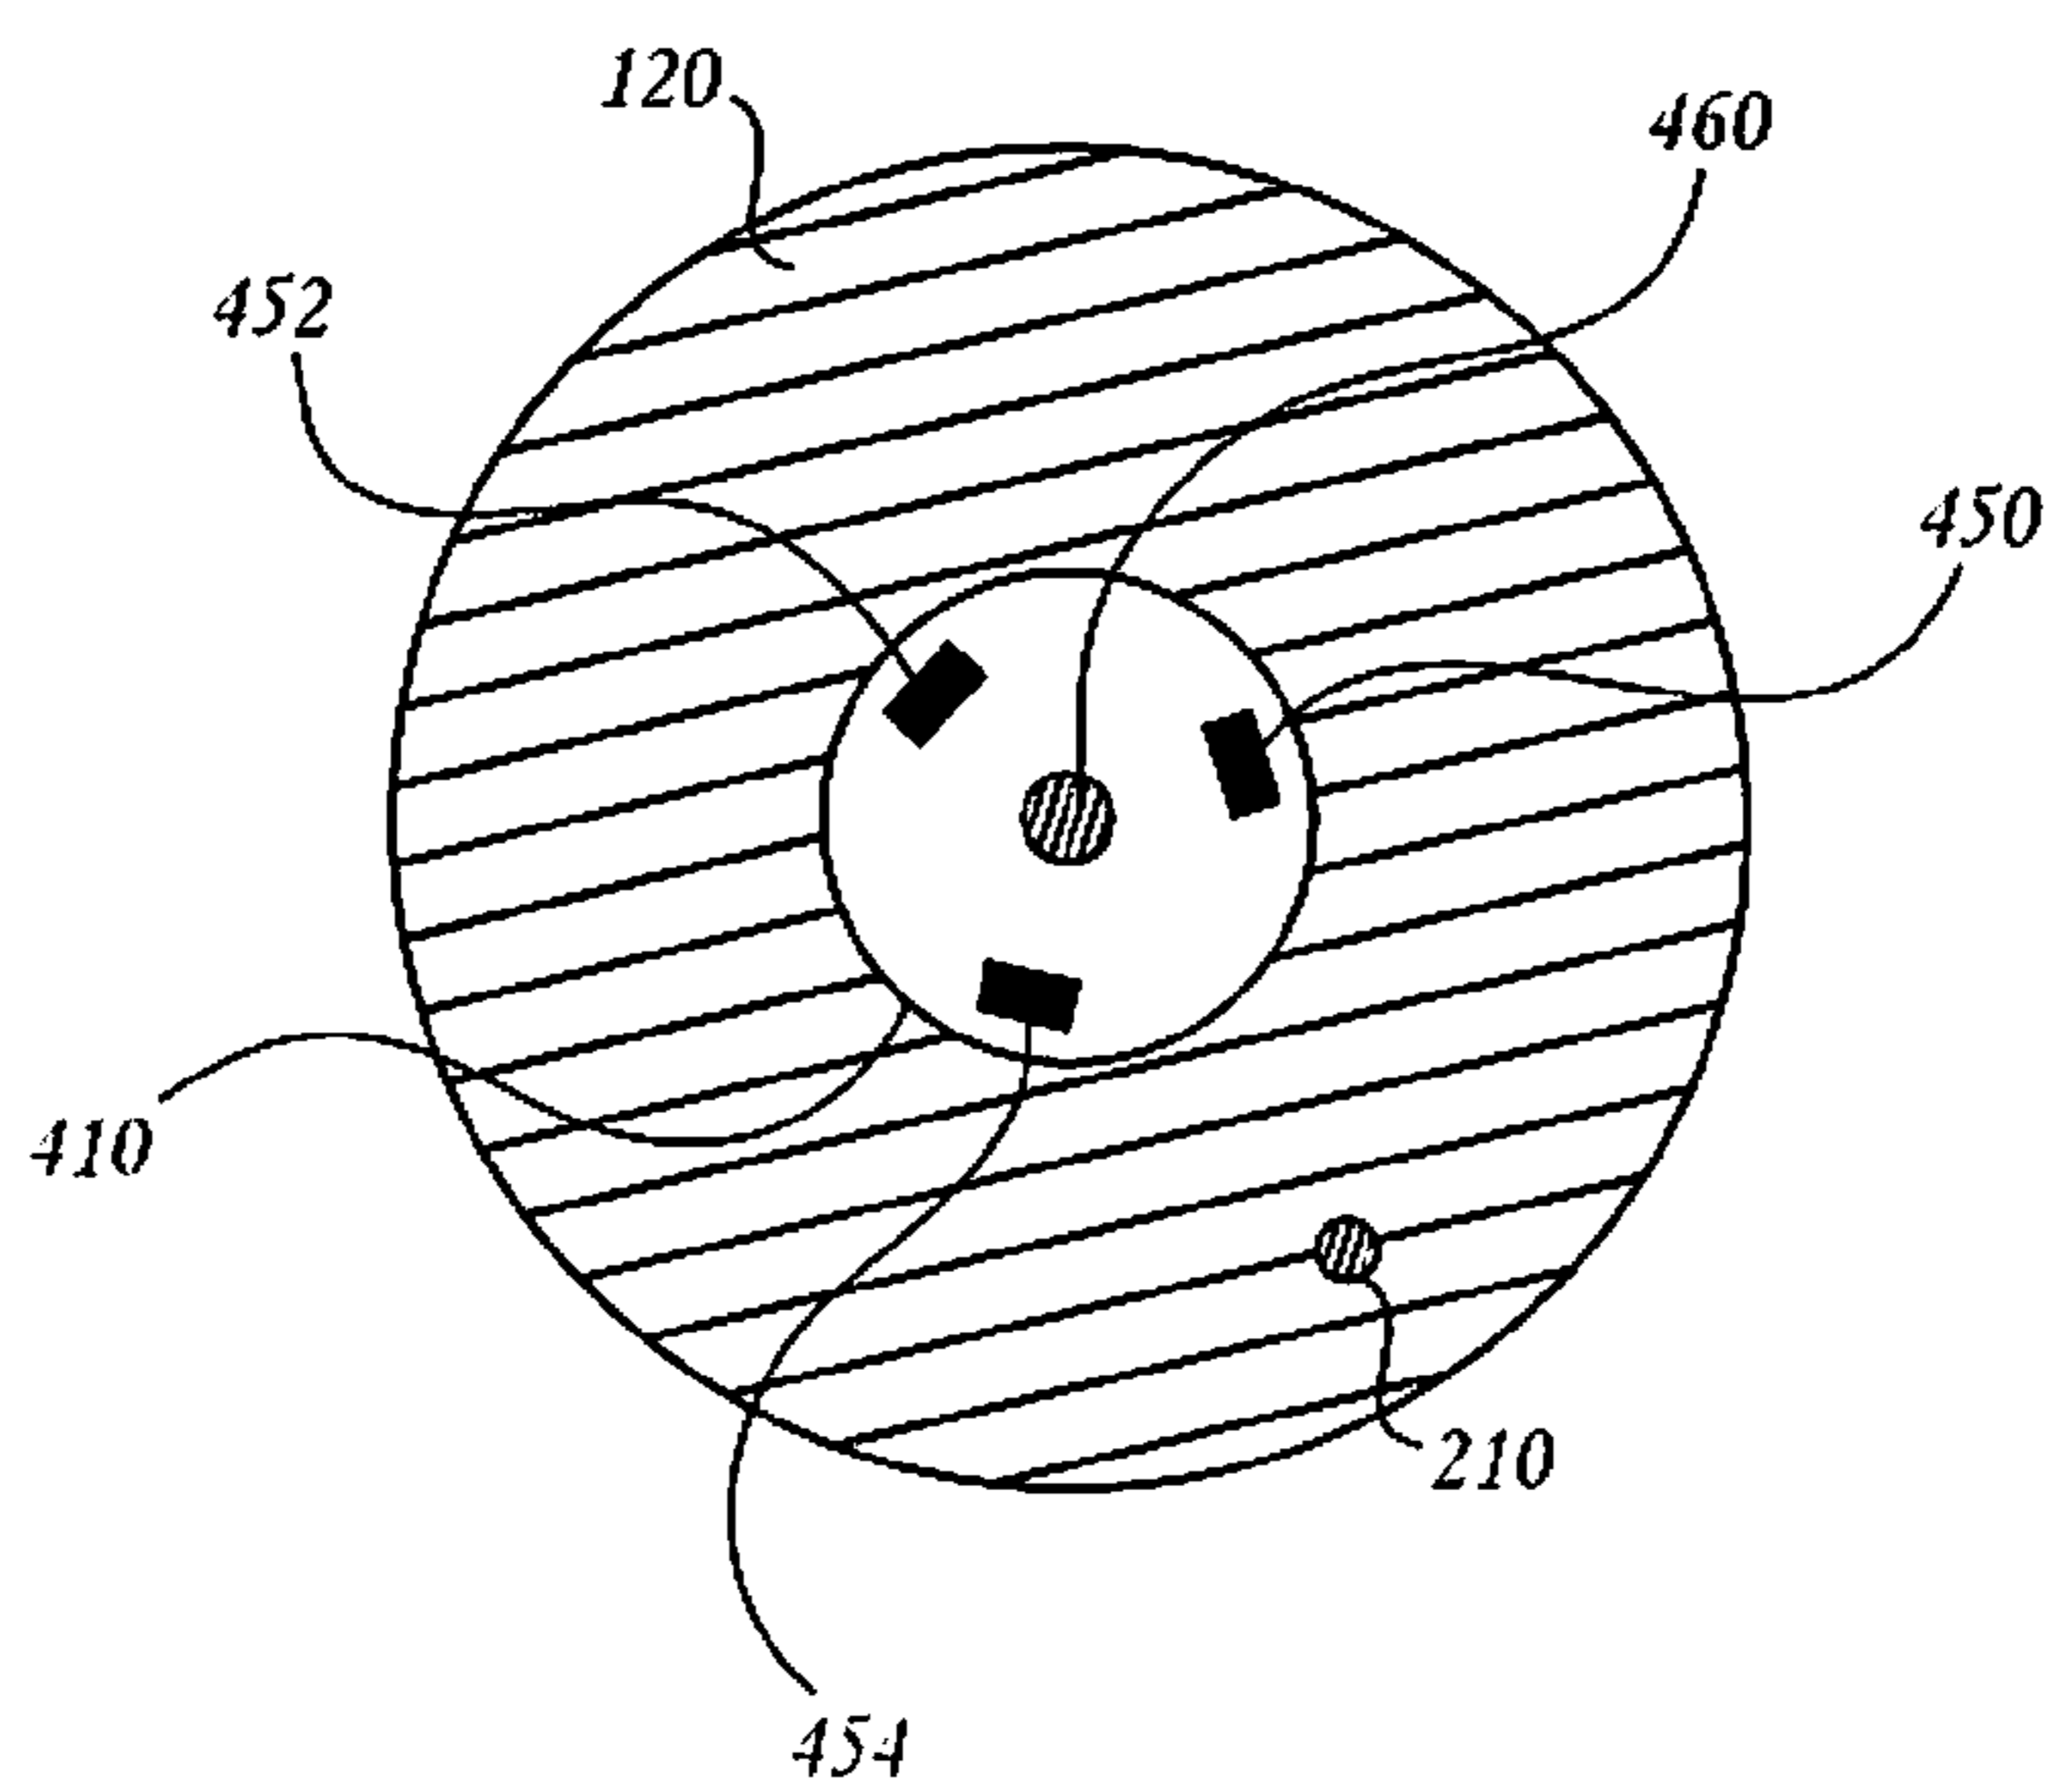


FIG. 4F

FIG. 5A

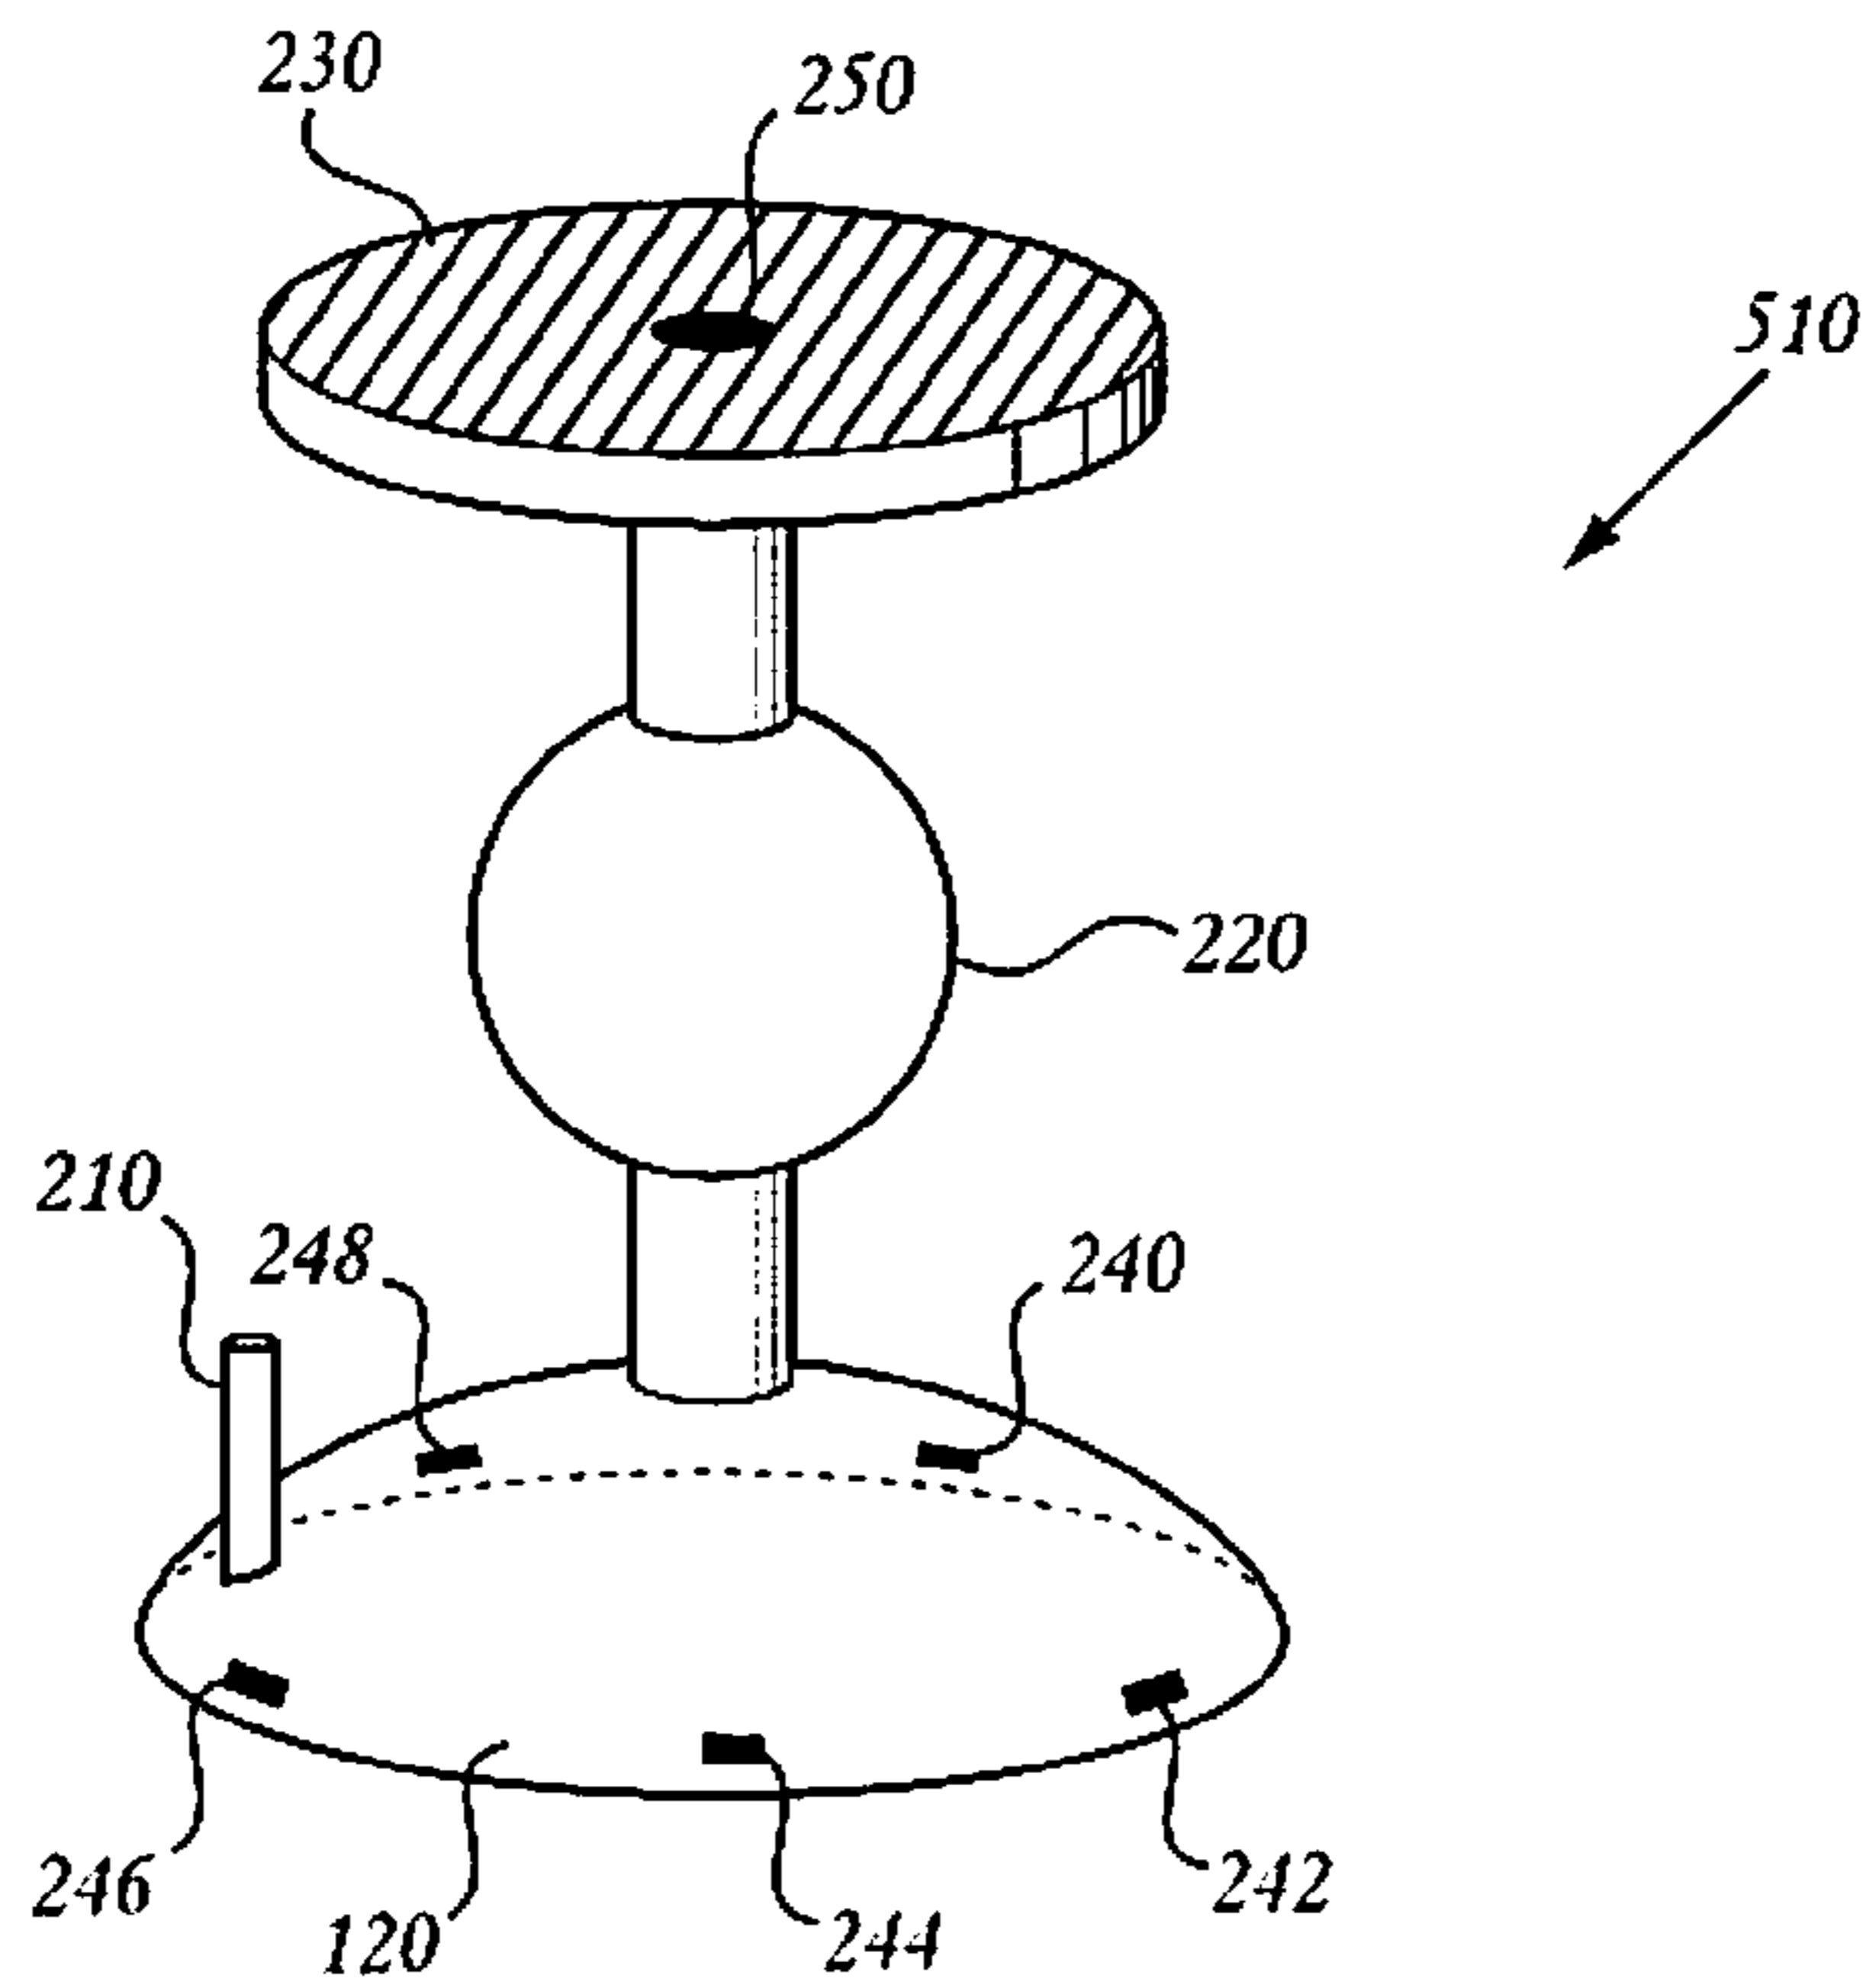


FIG. 5B

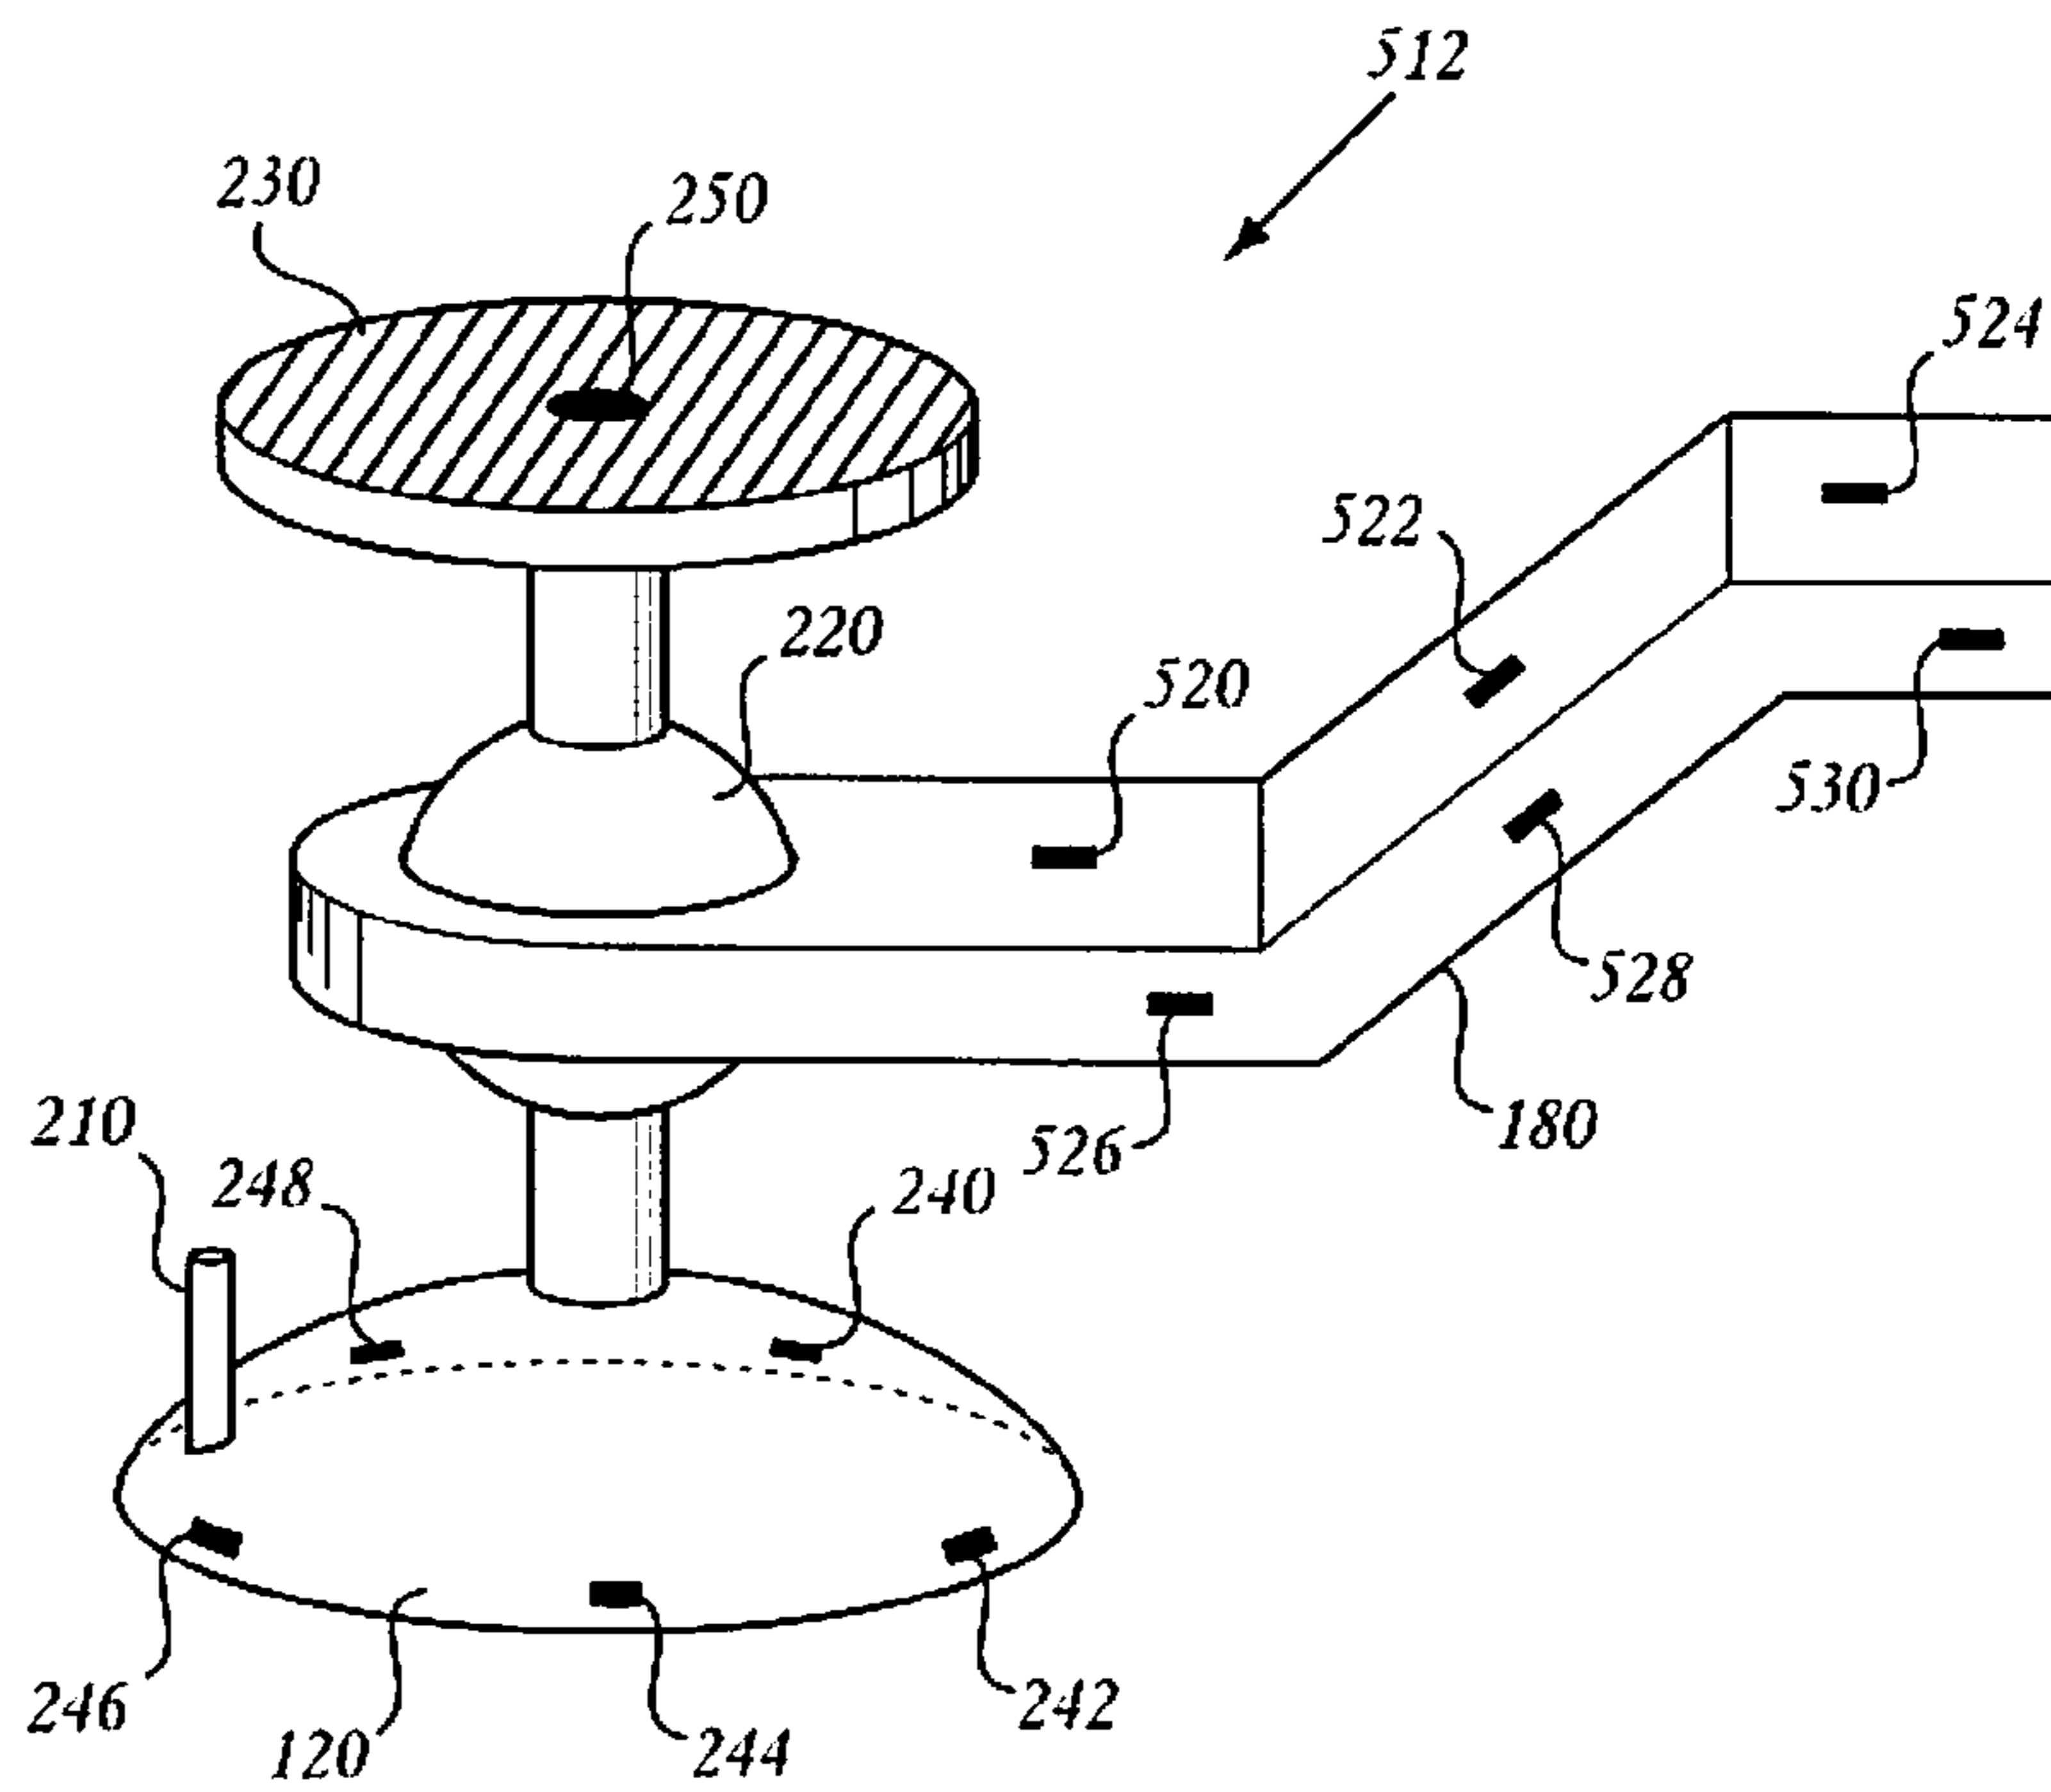


FIG. 6A

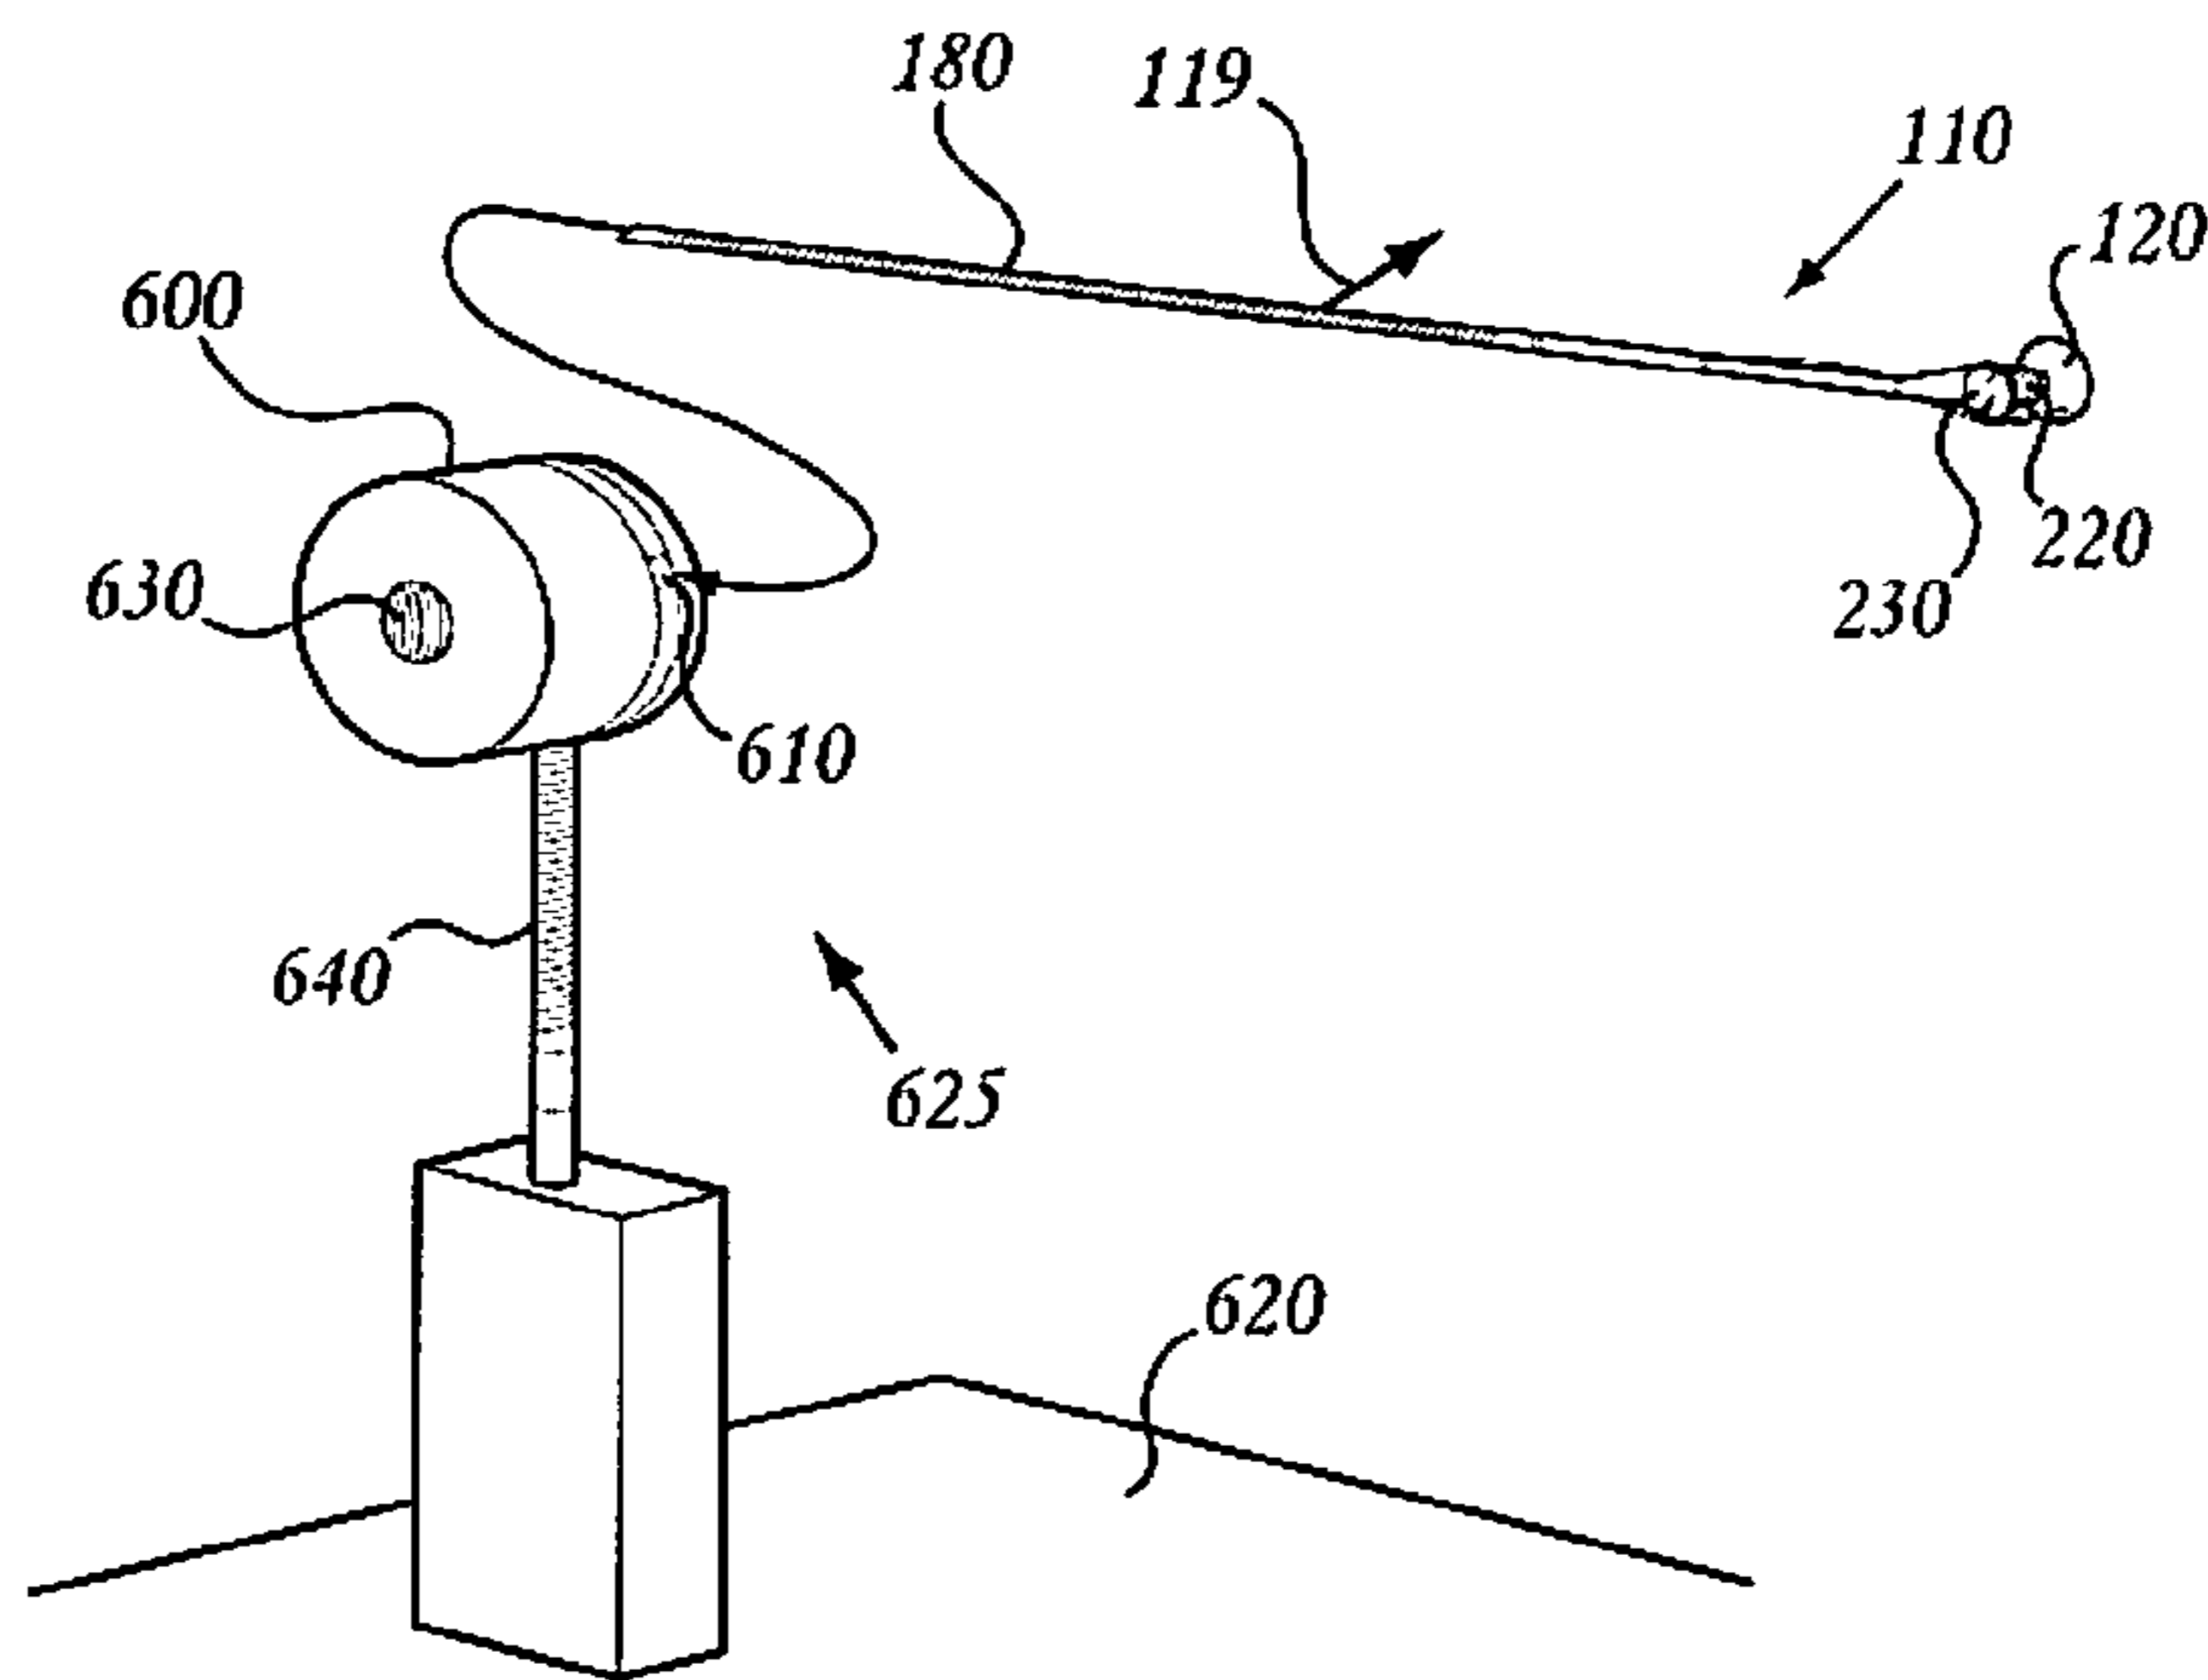


FIG. 6B

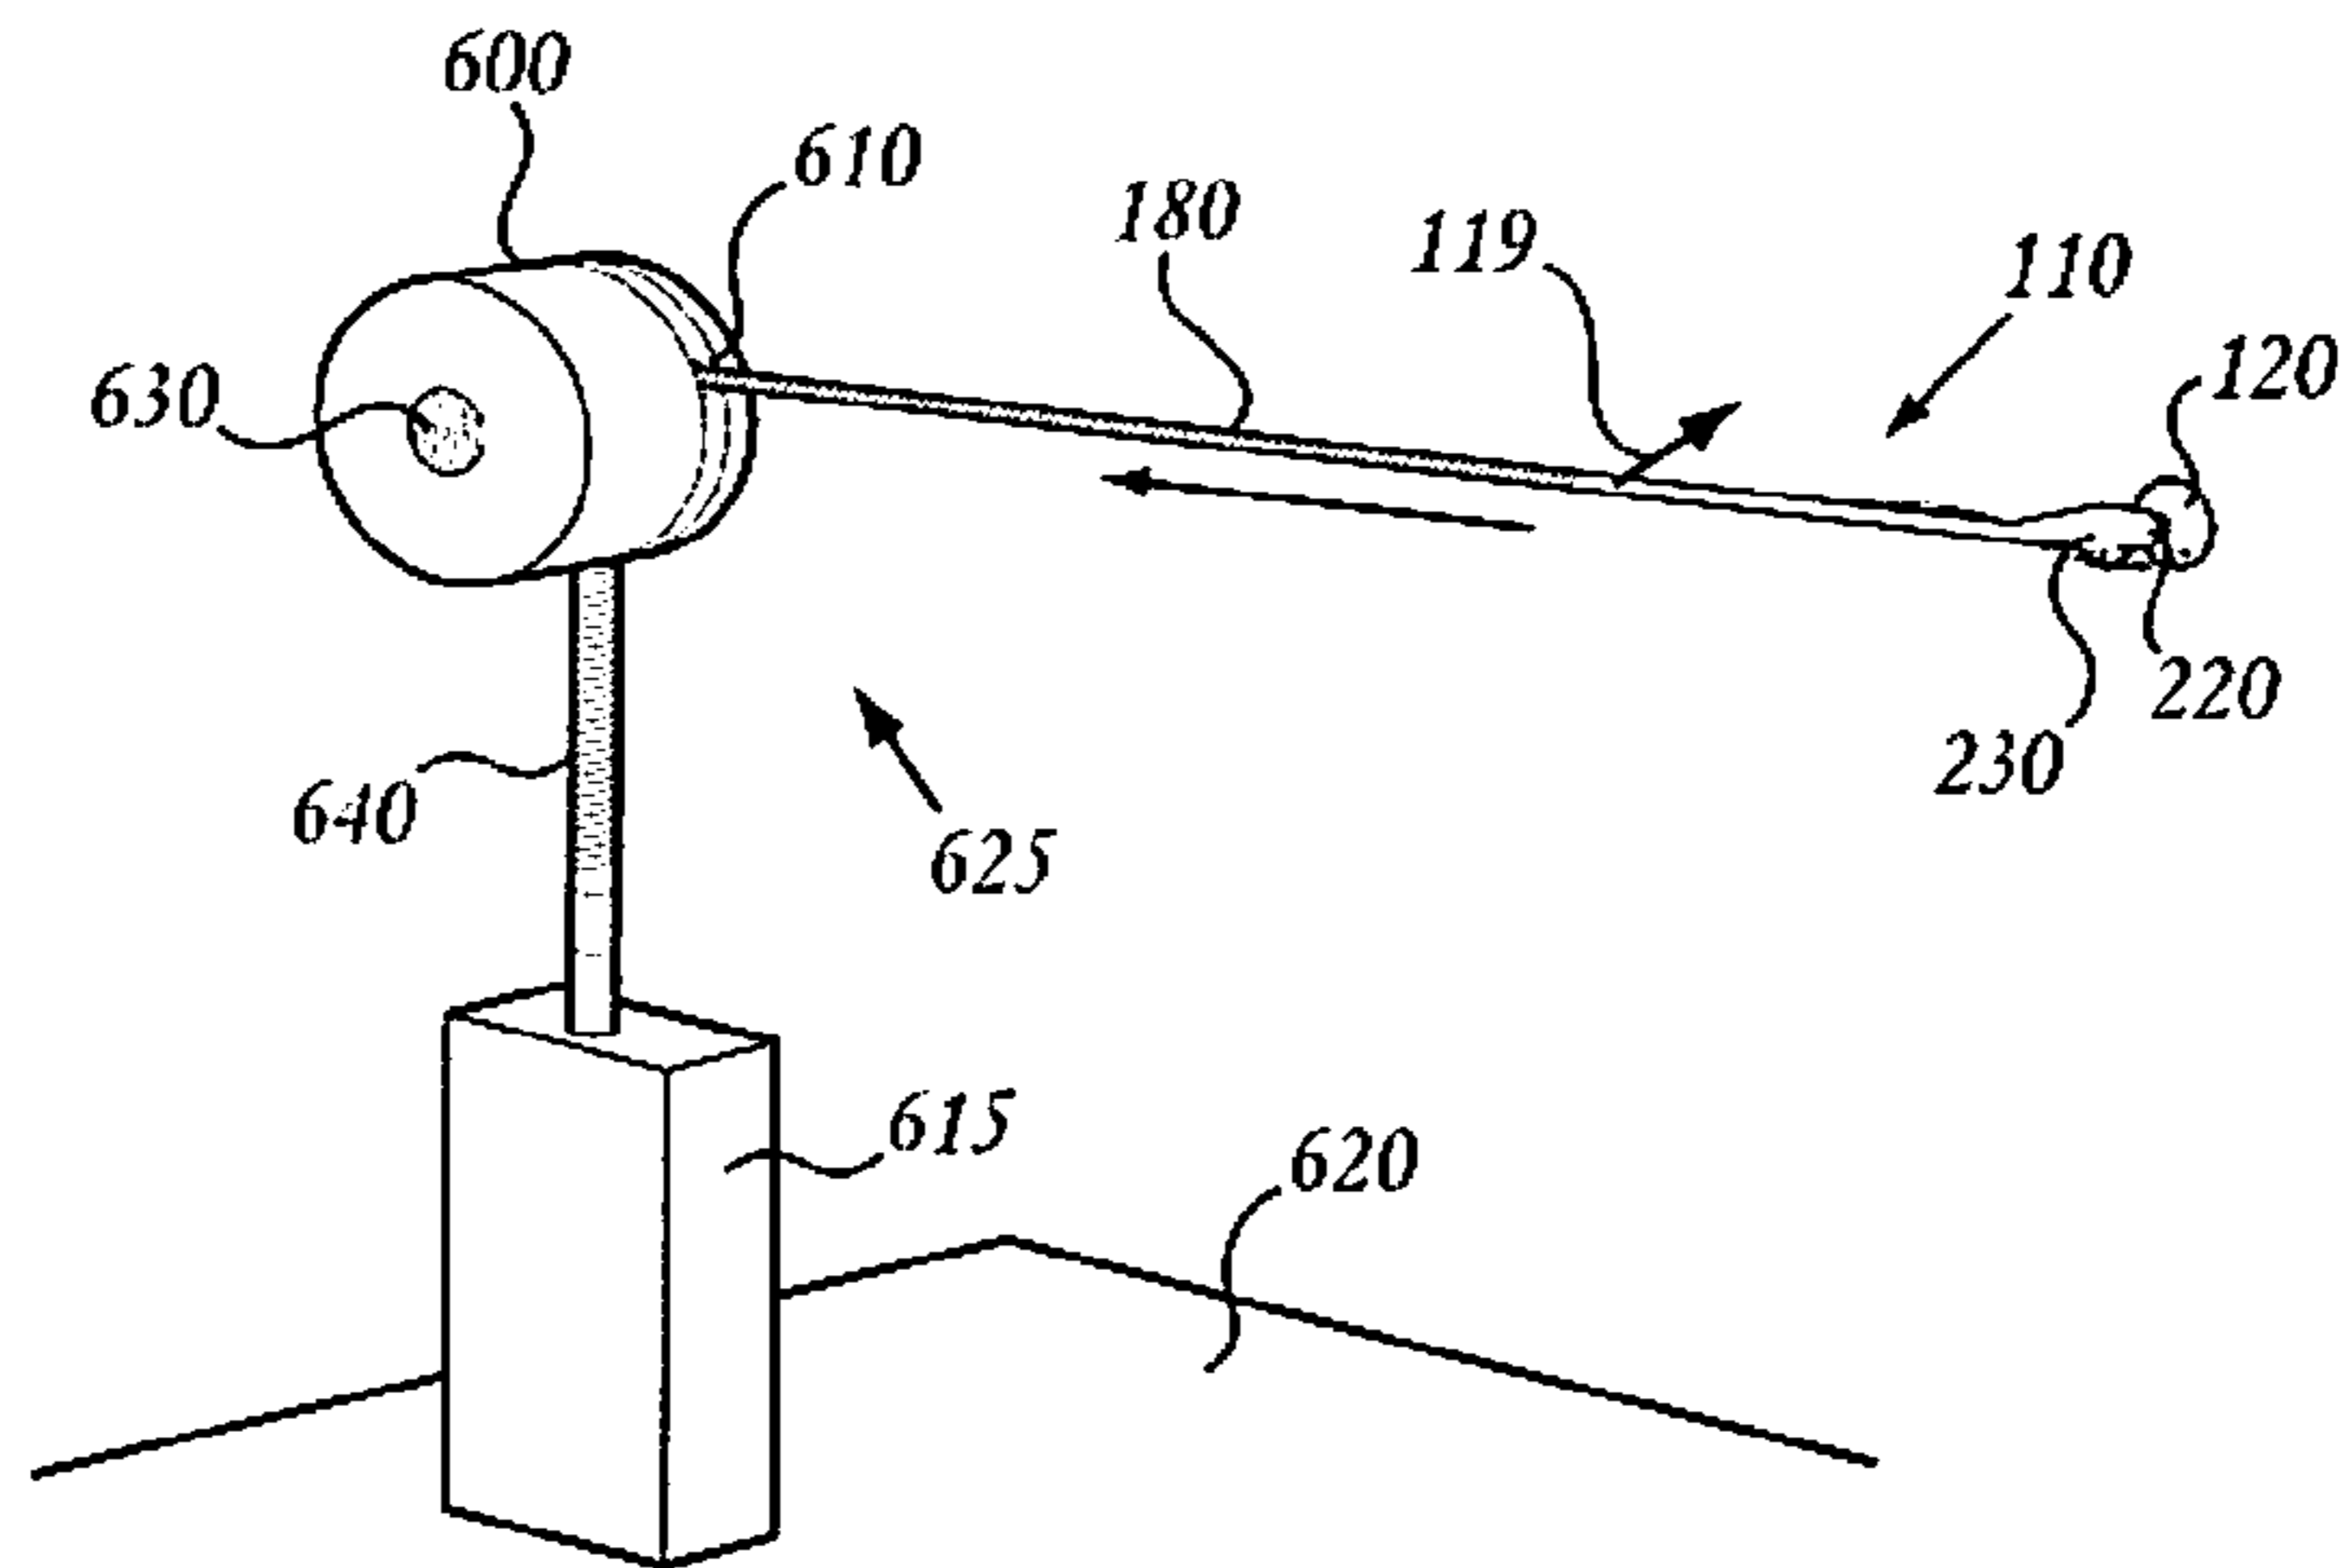
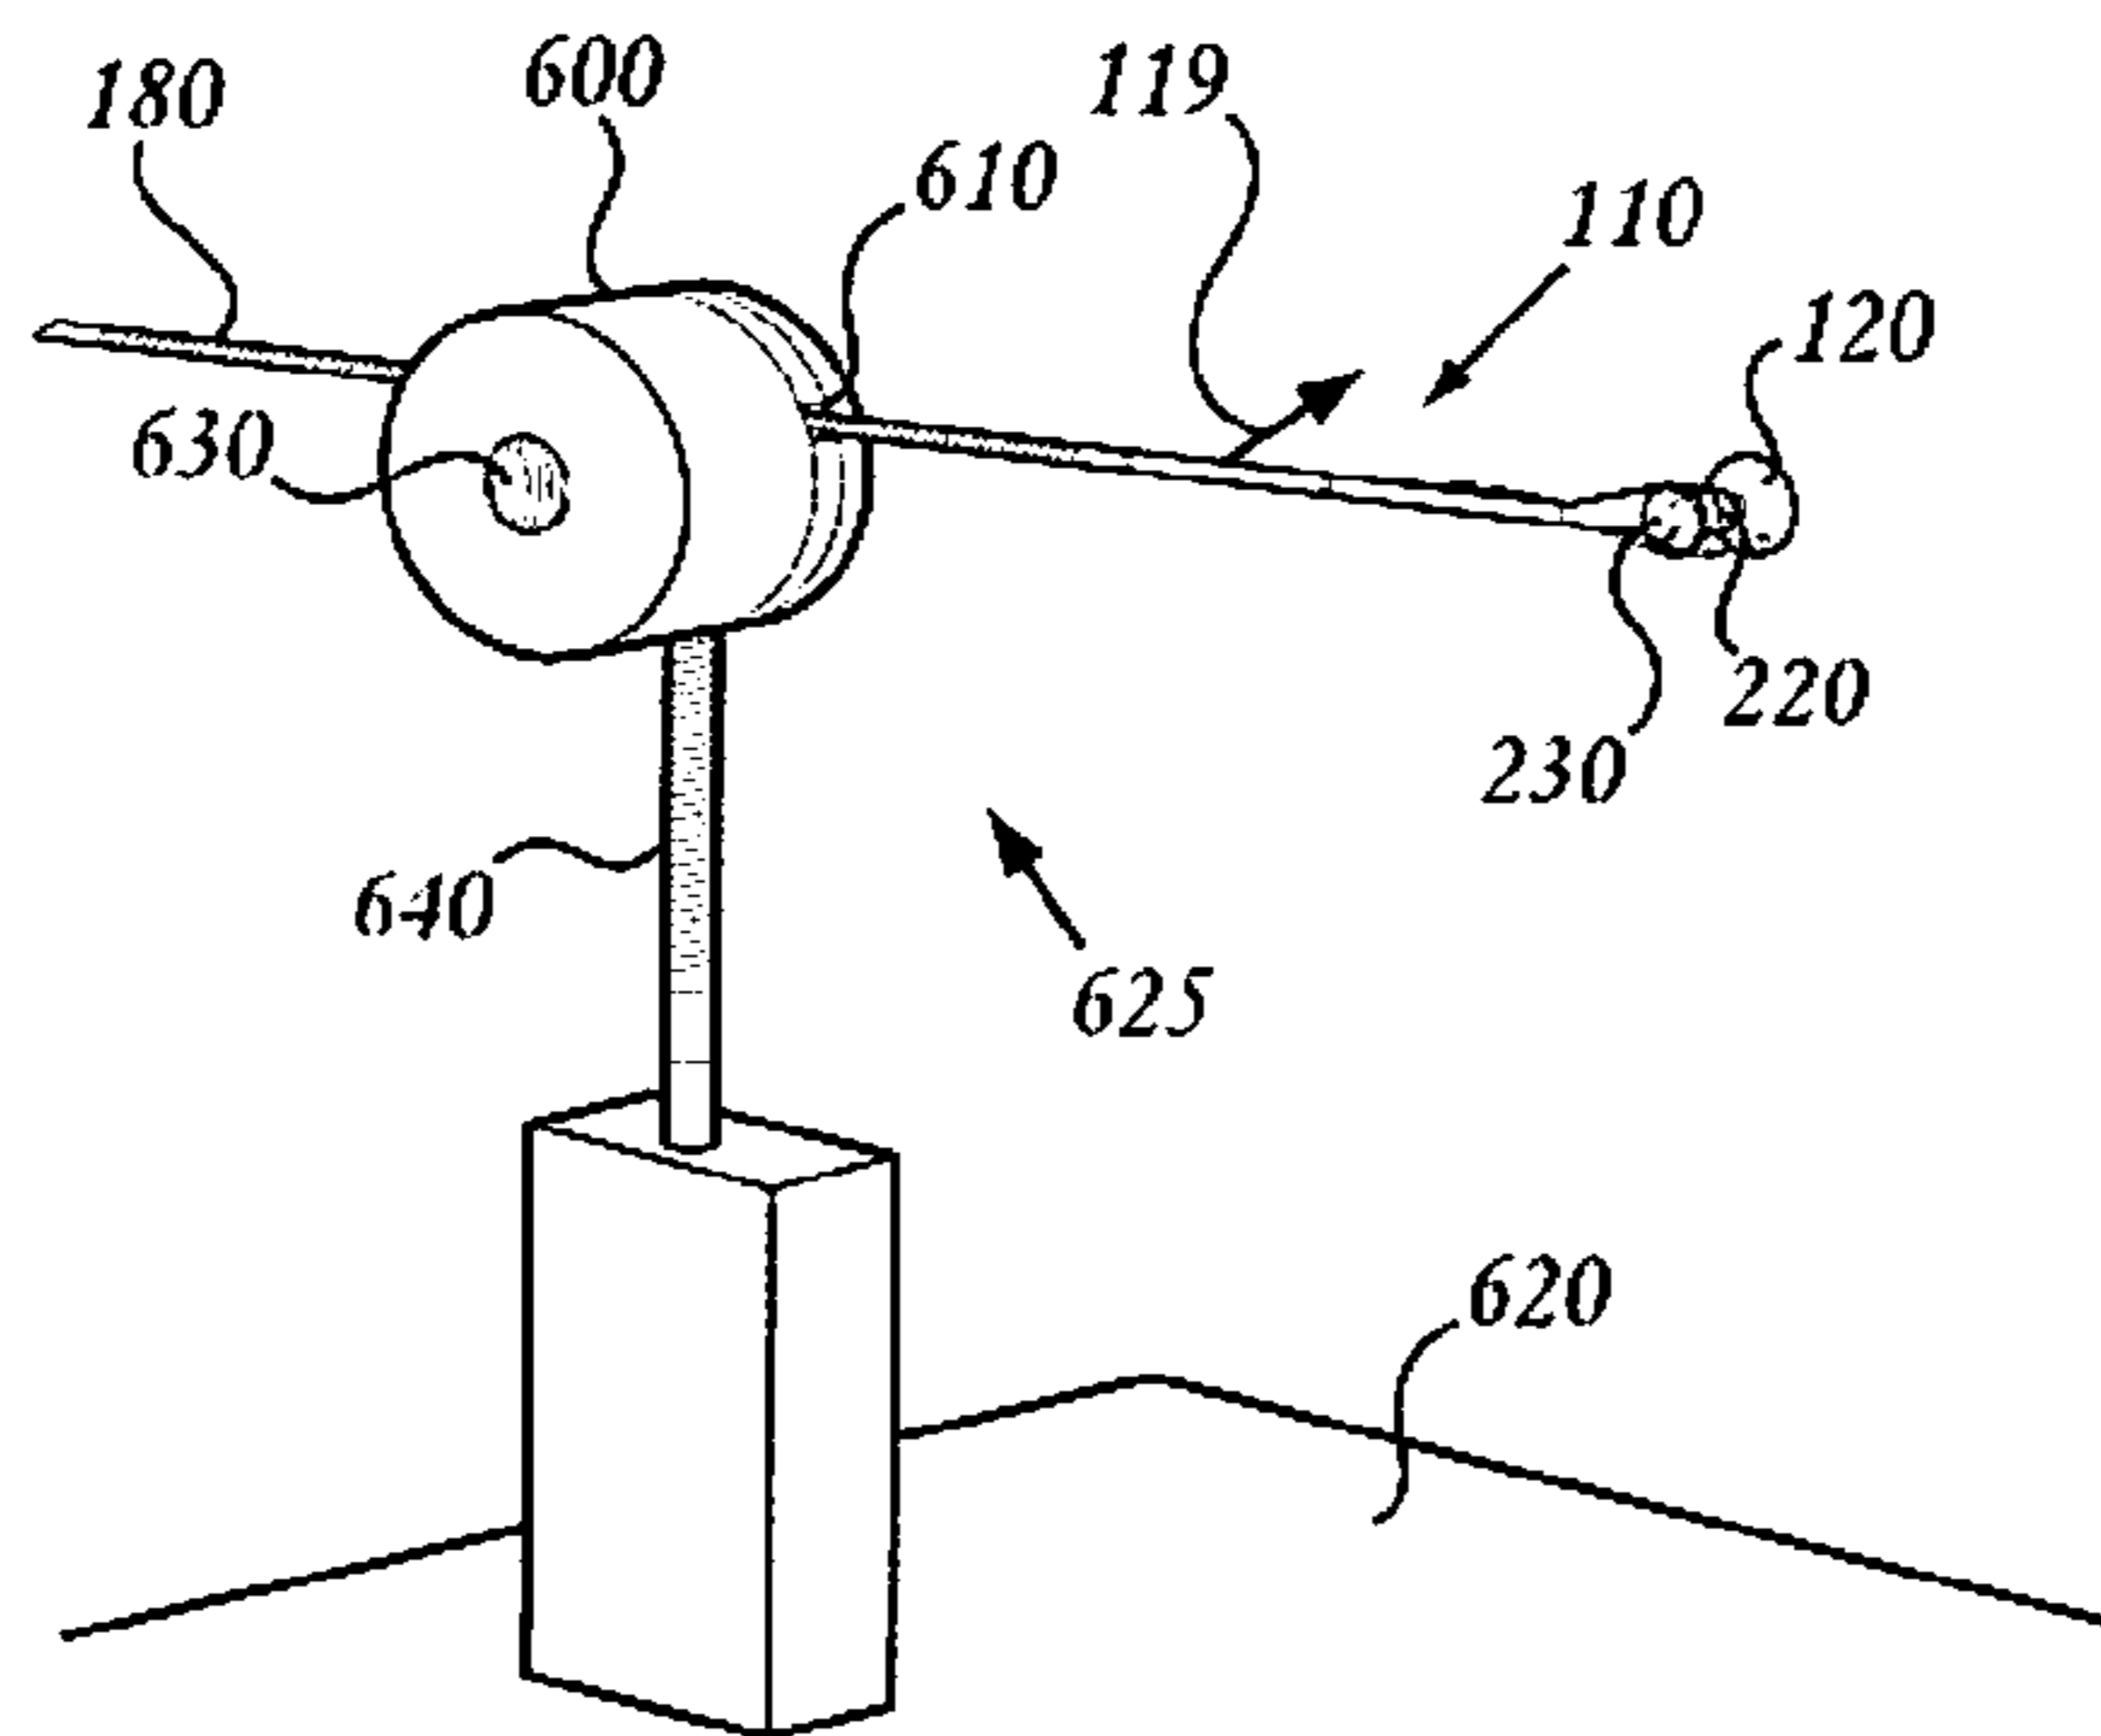


FIG. 6C



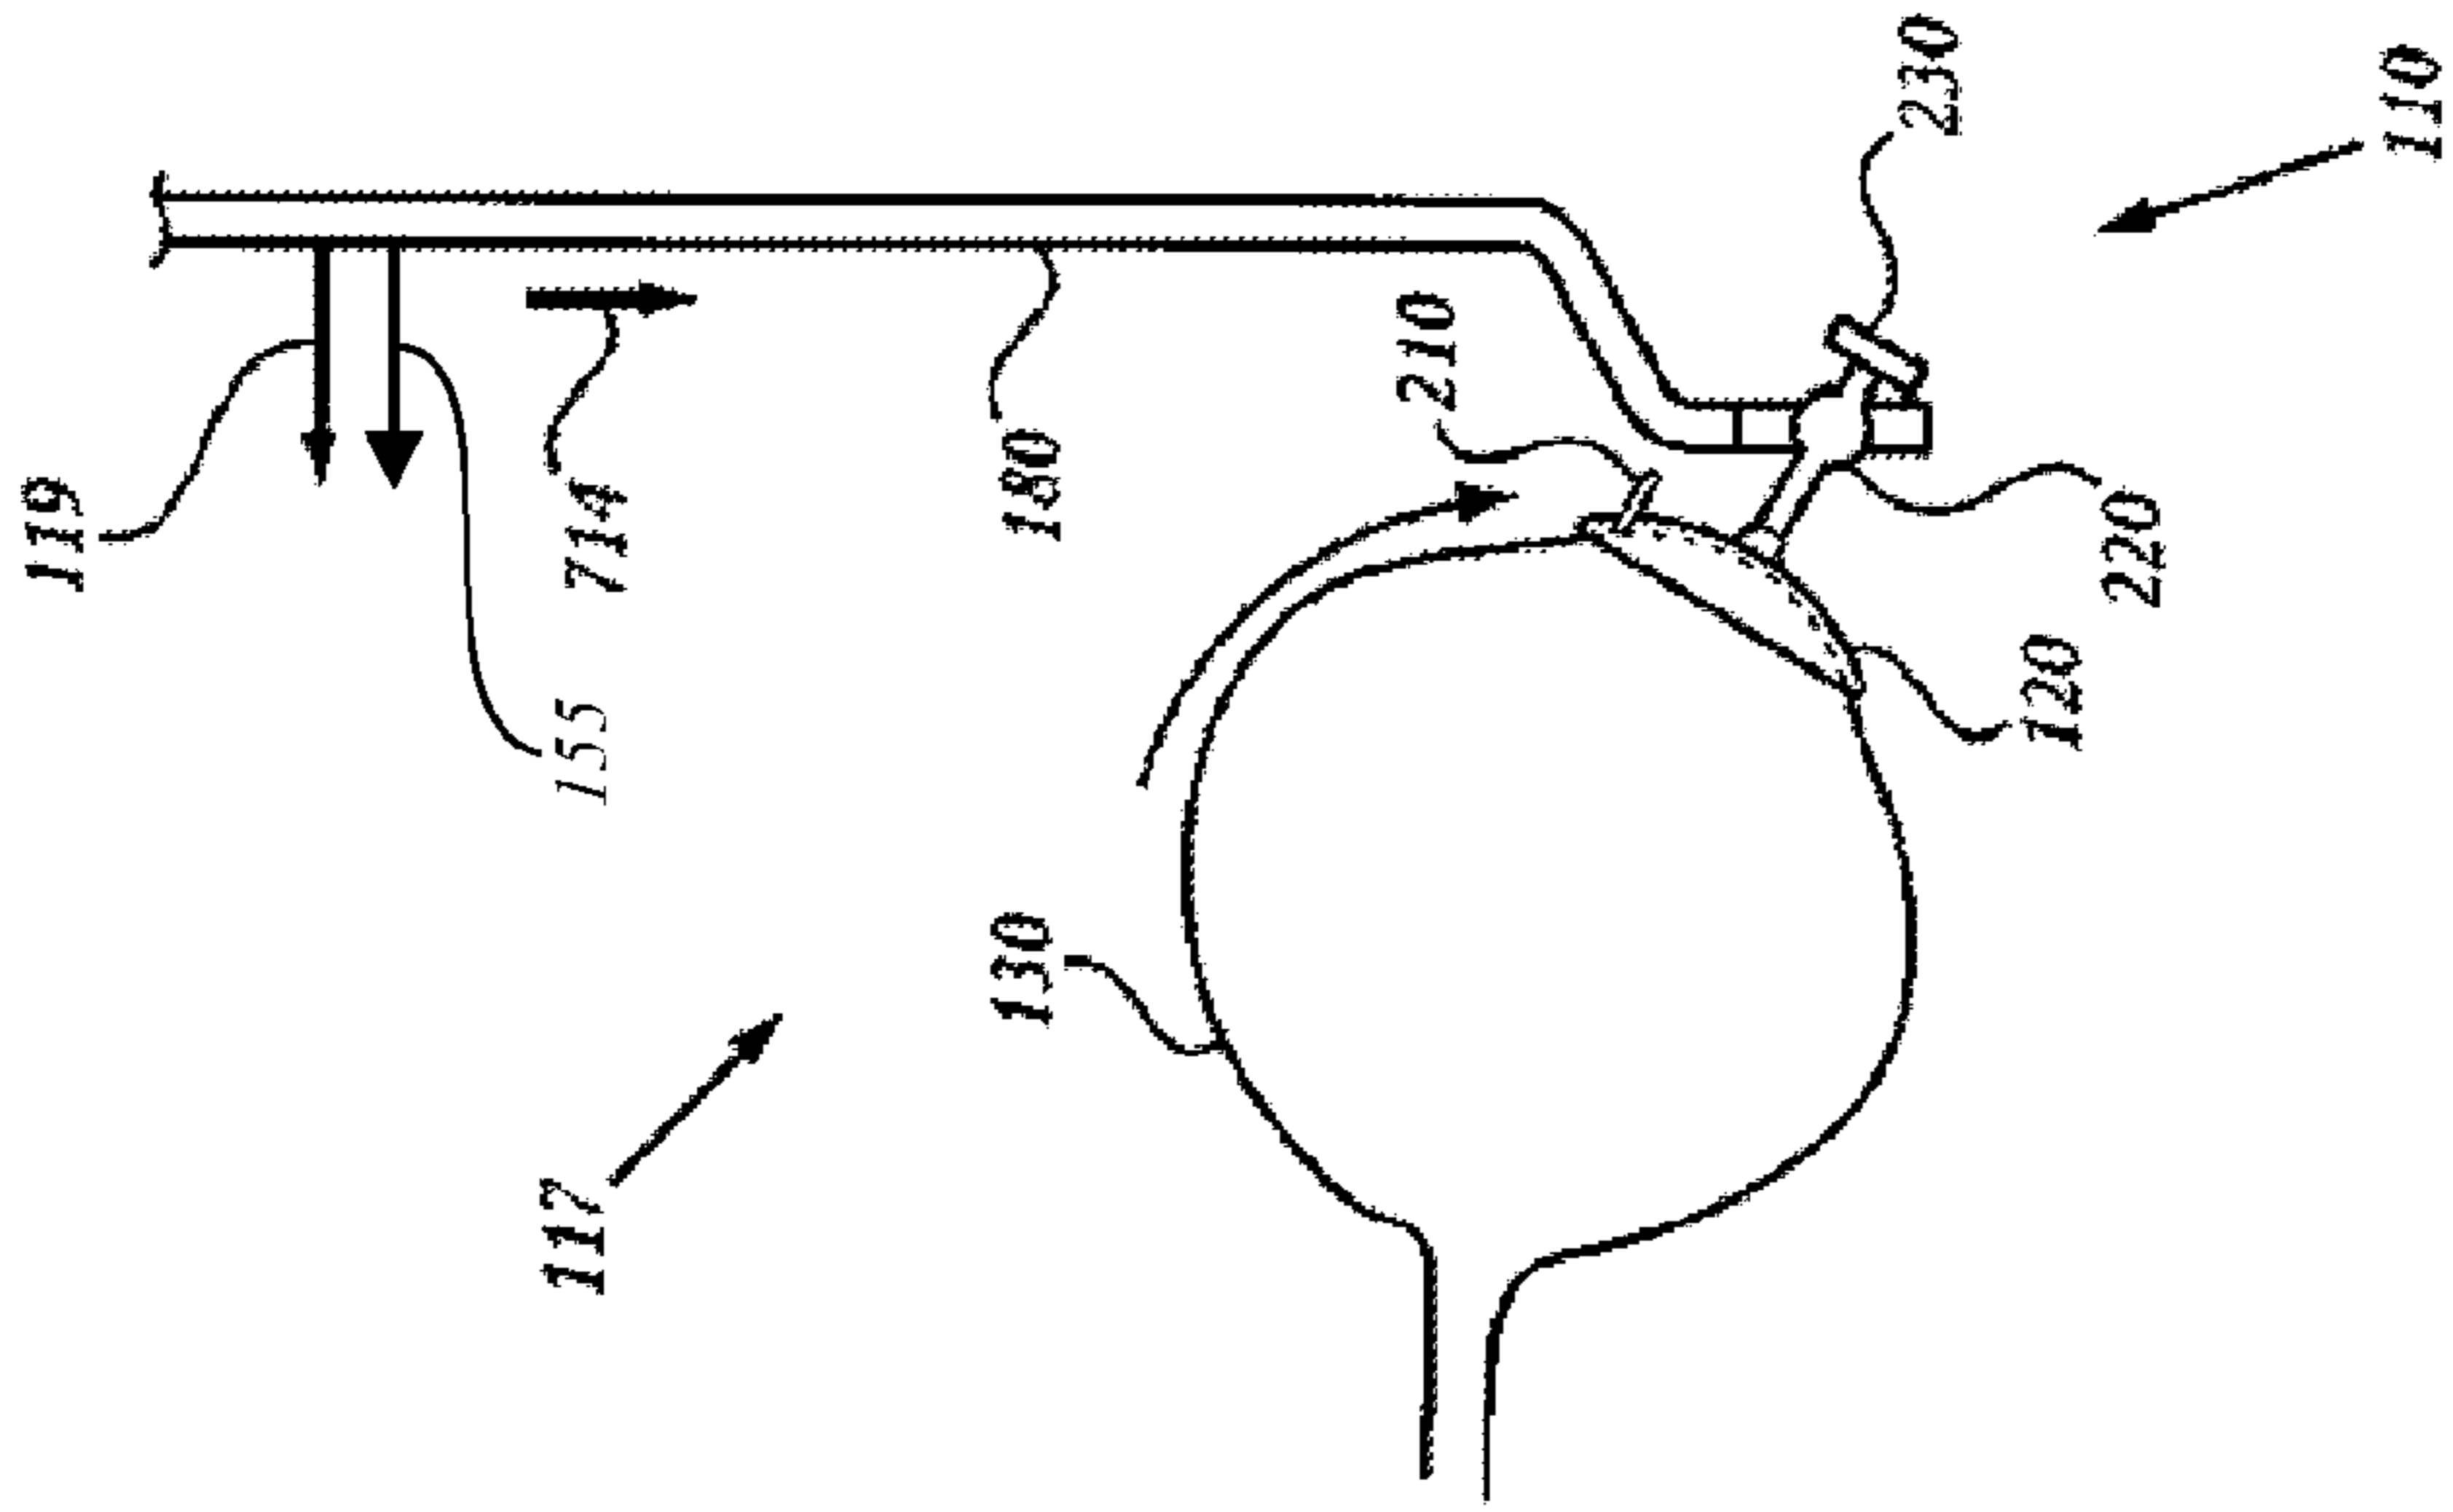


FIG. 7A

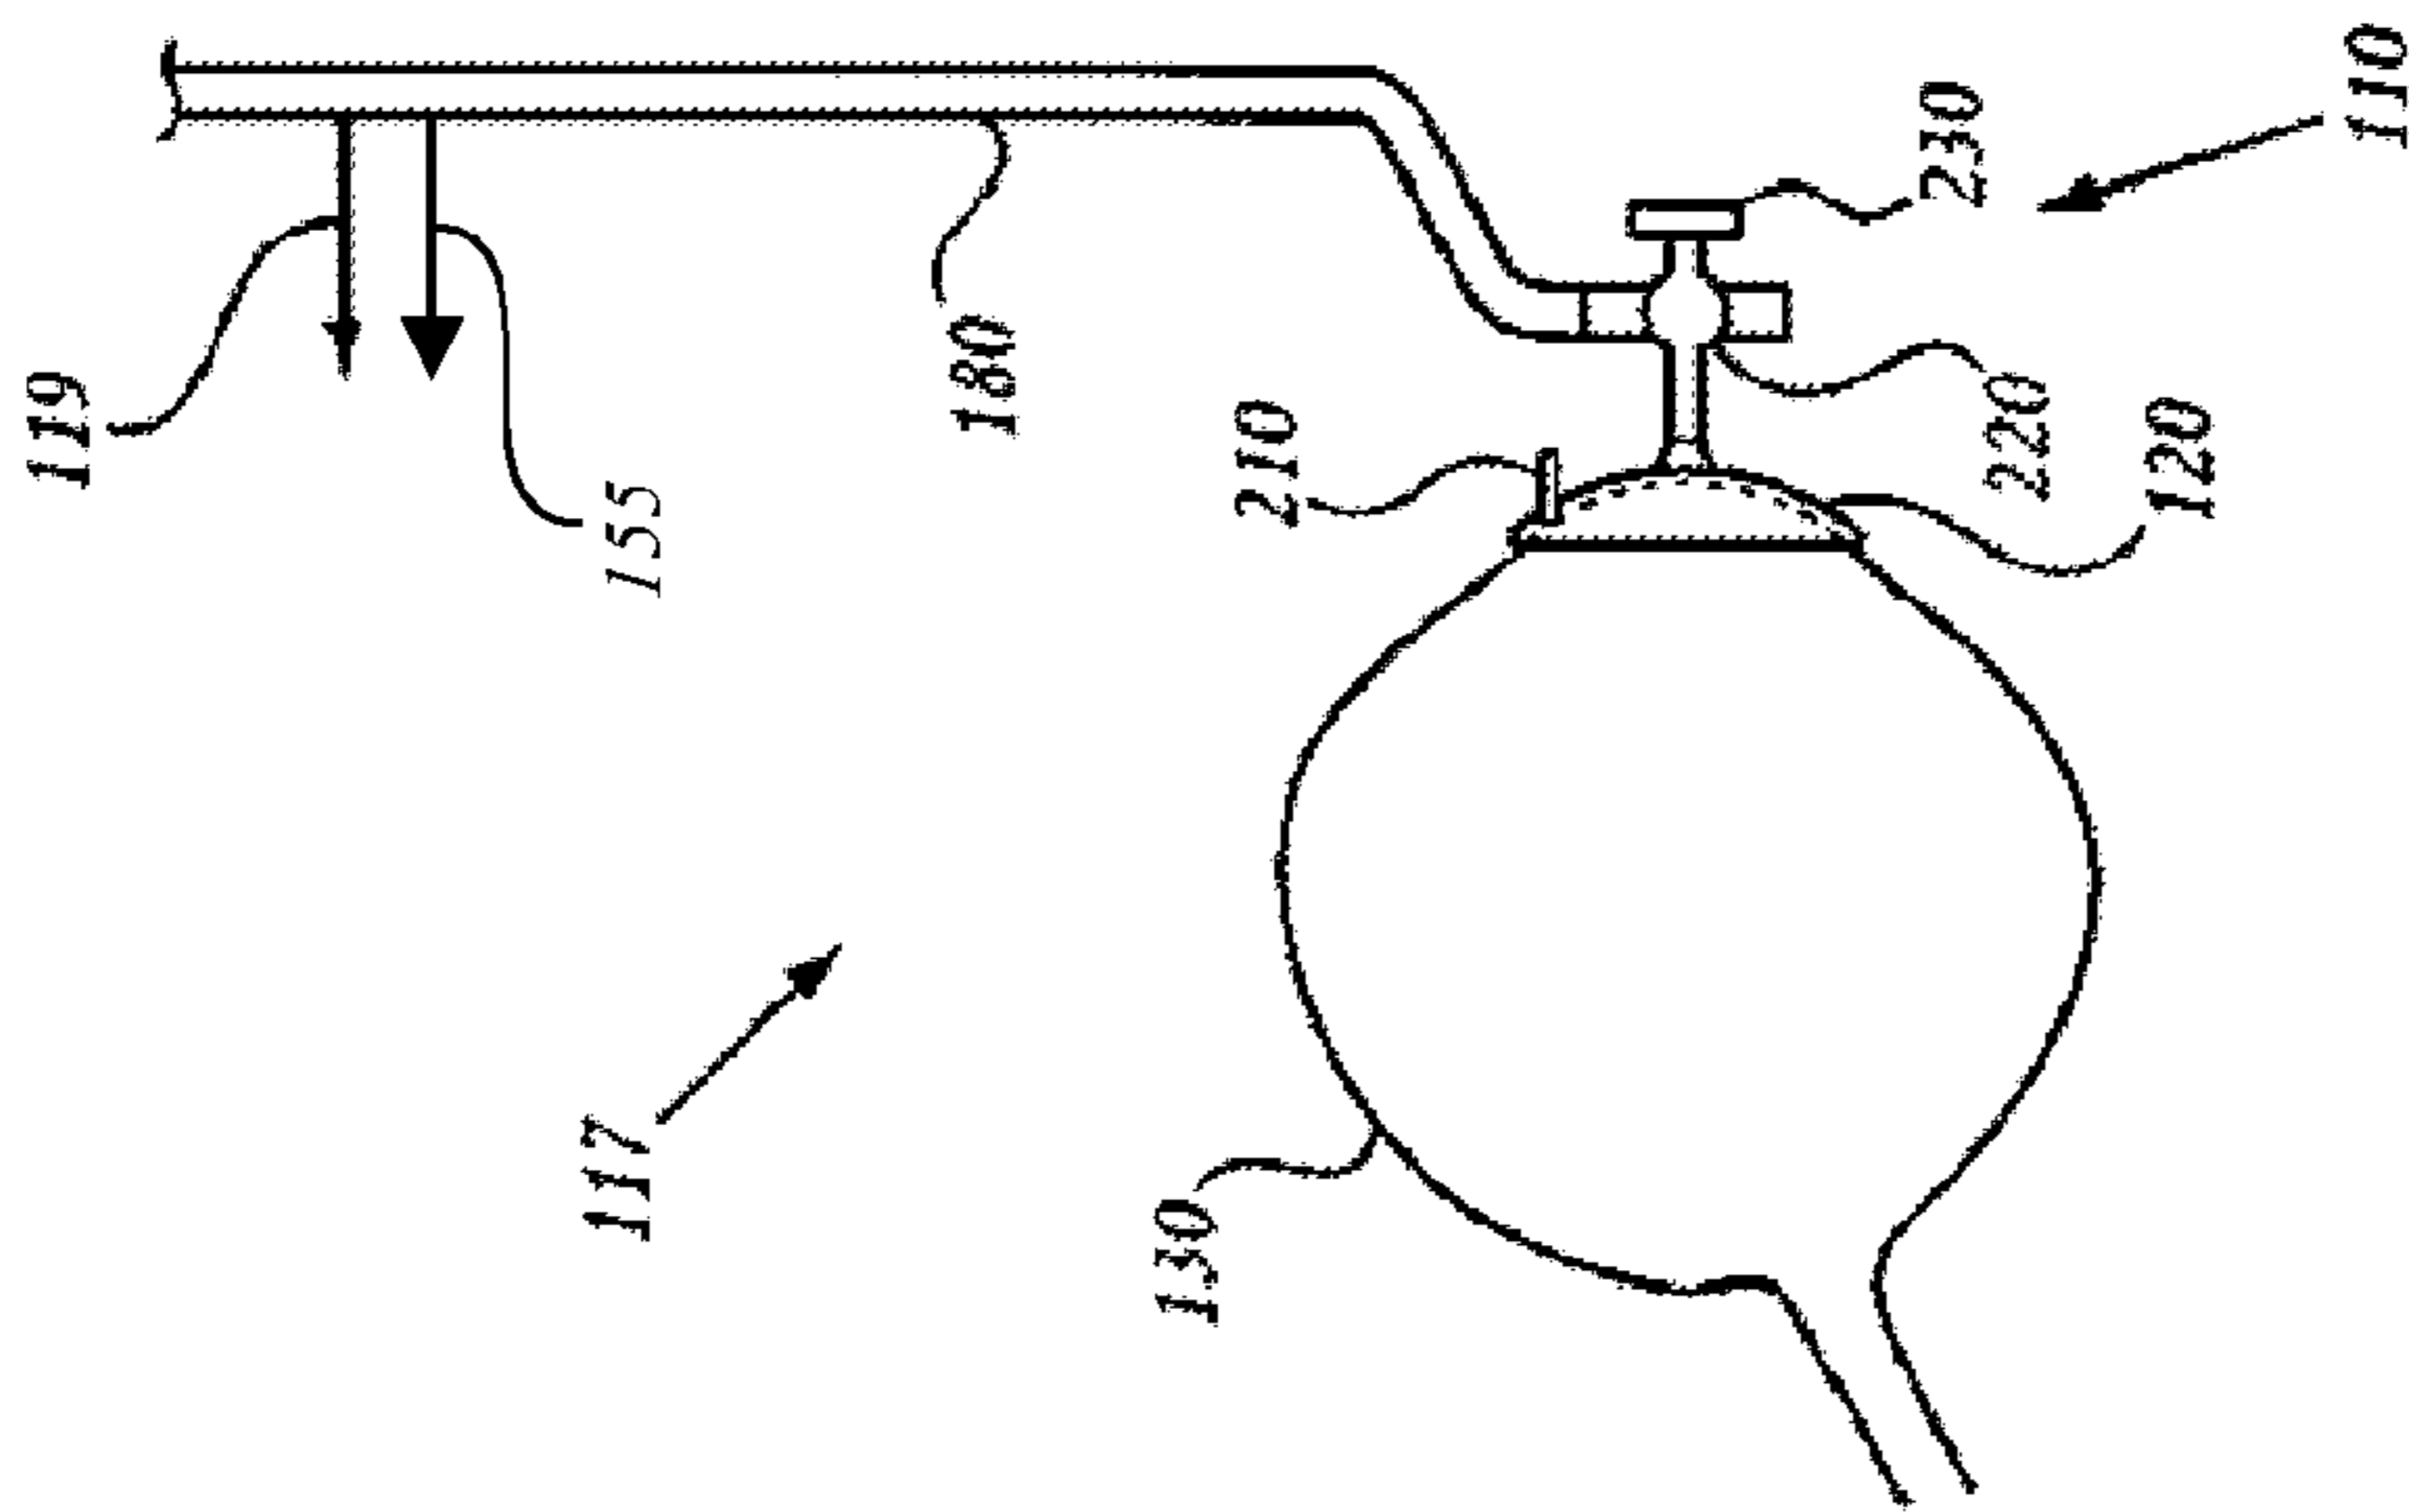


FIG. 7B

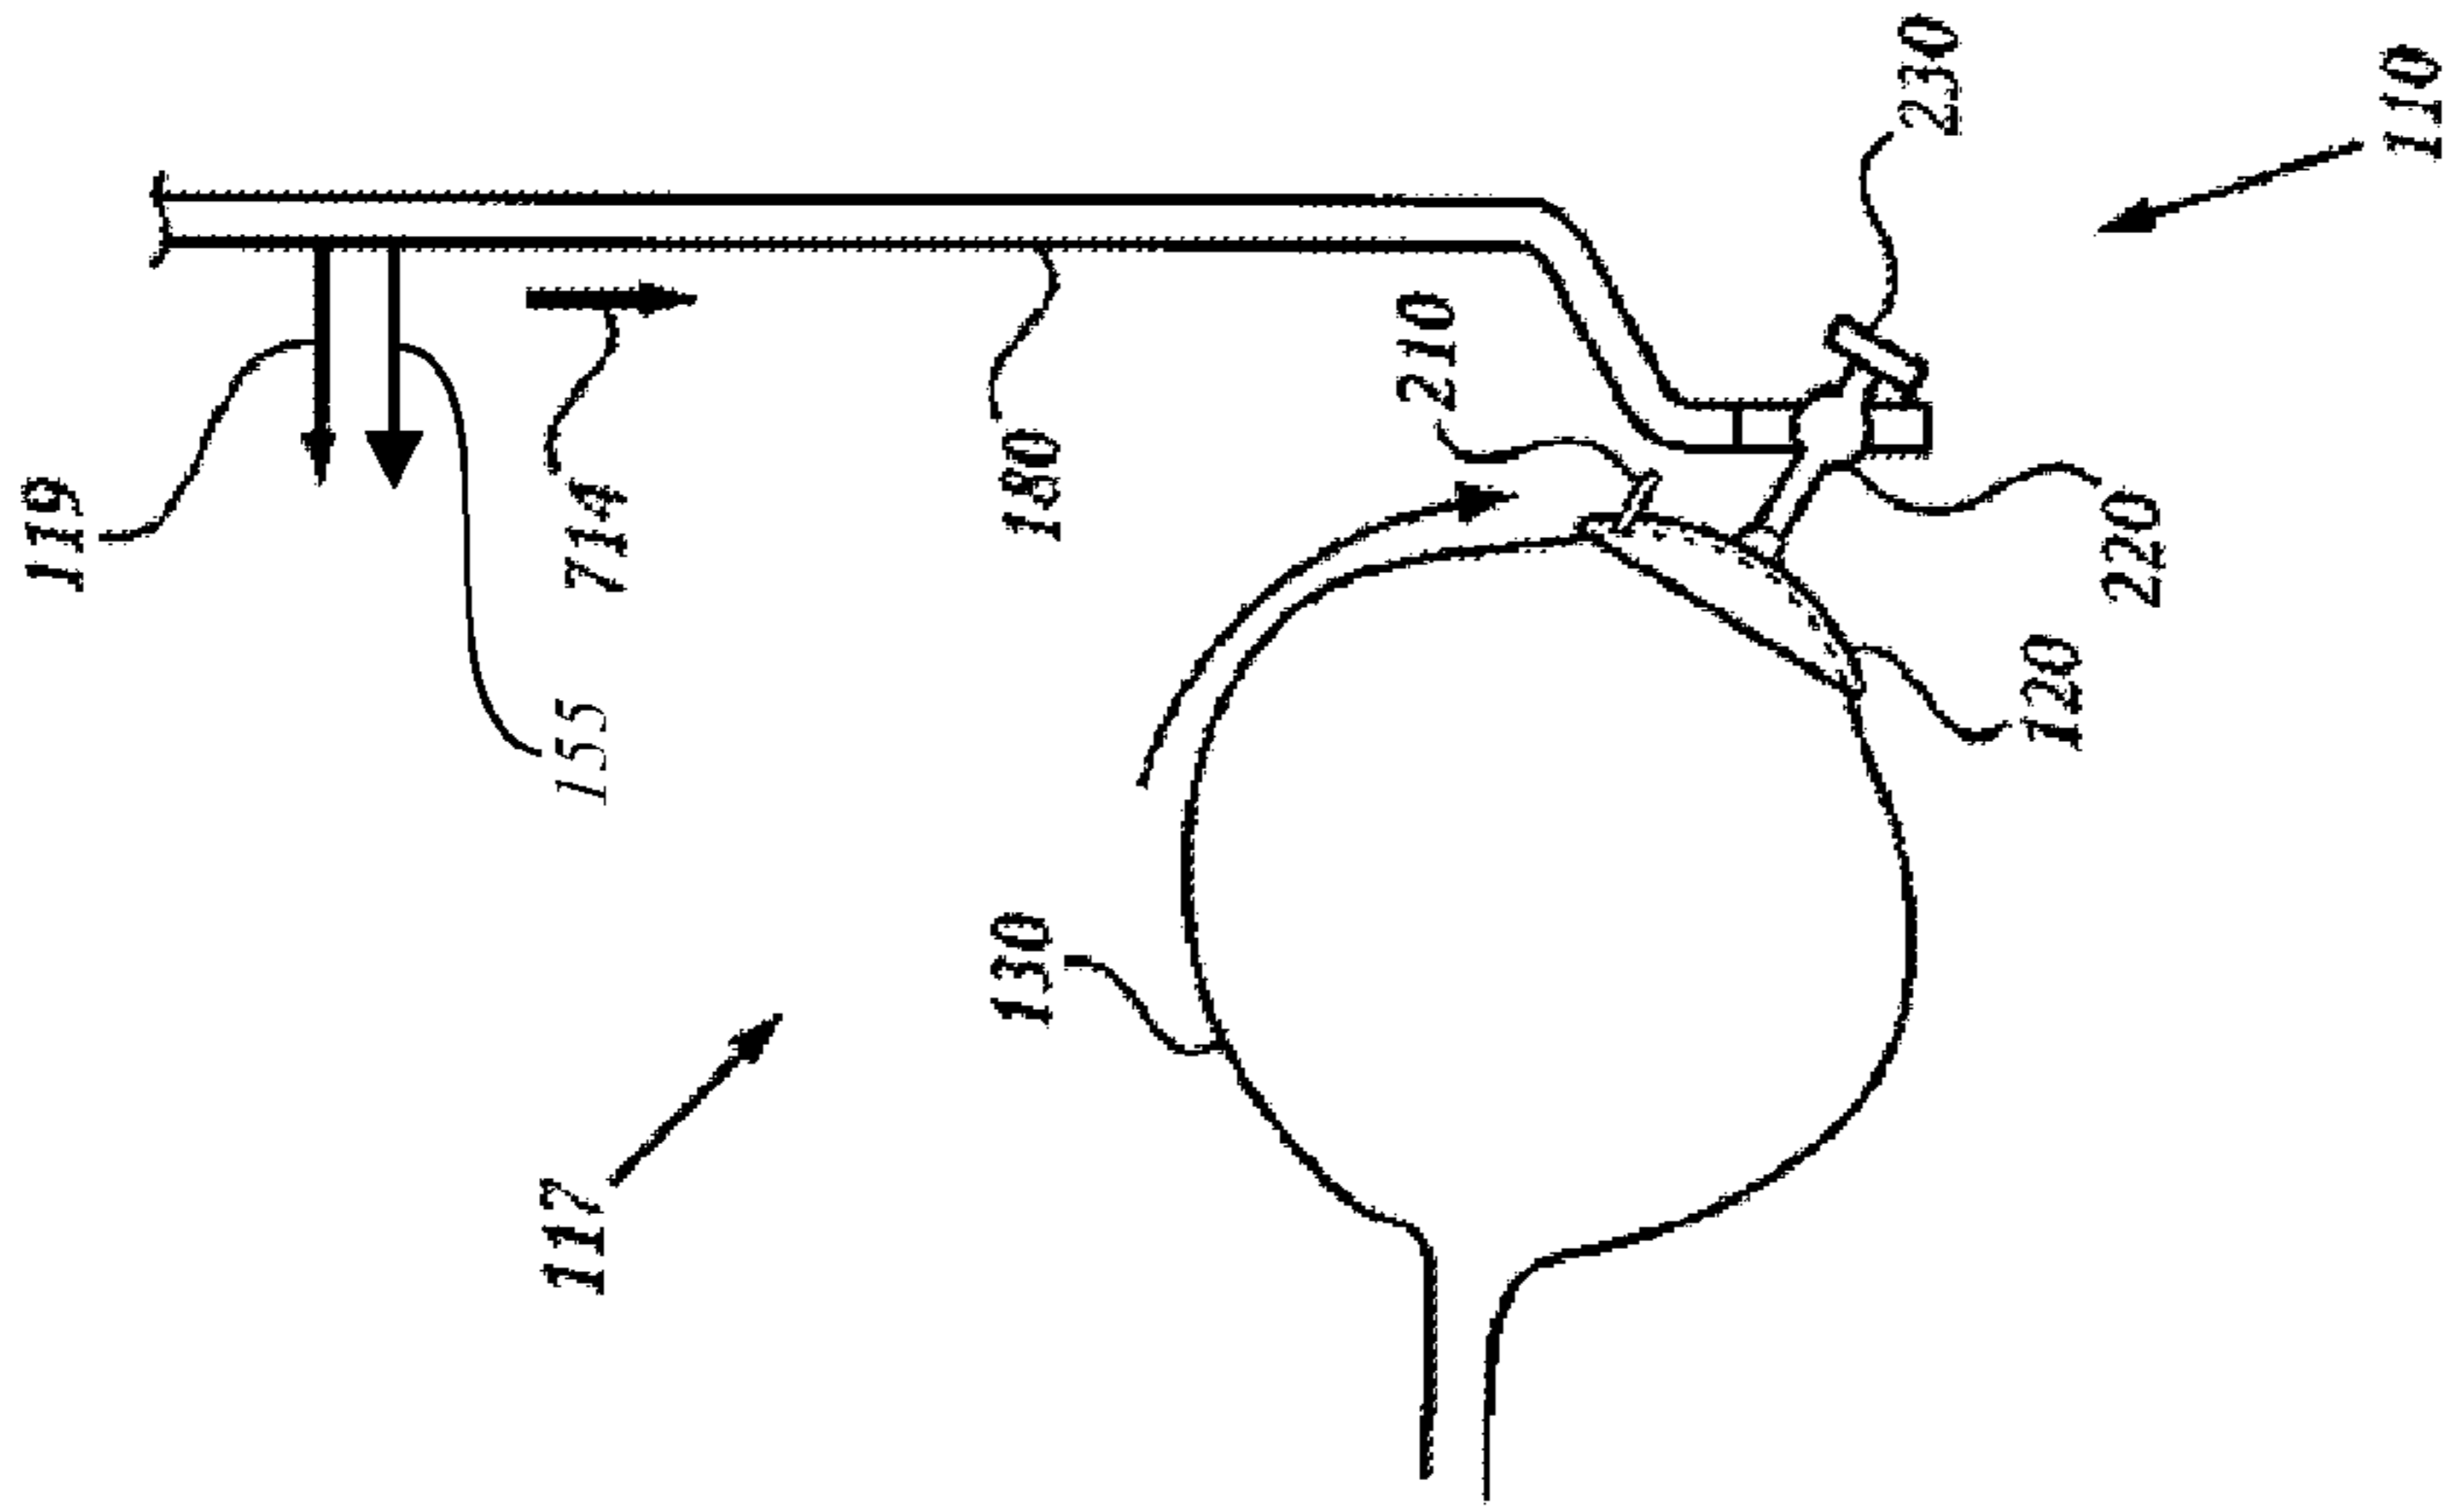


FIG. 7C

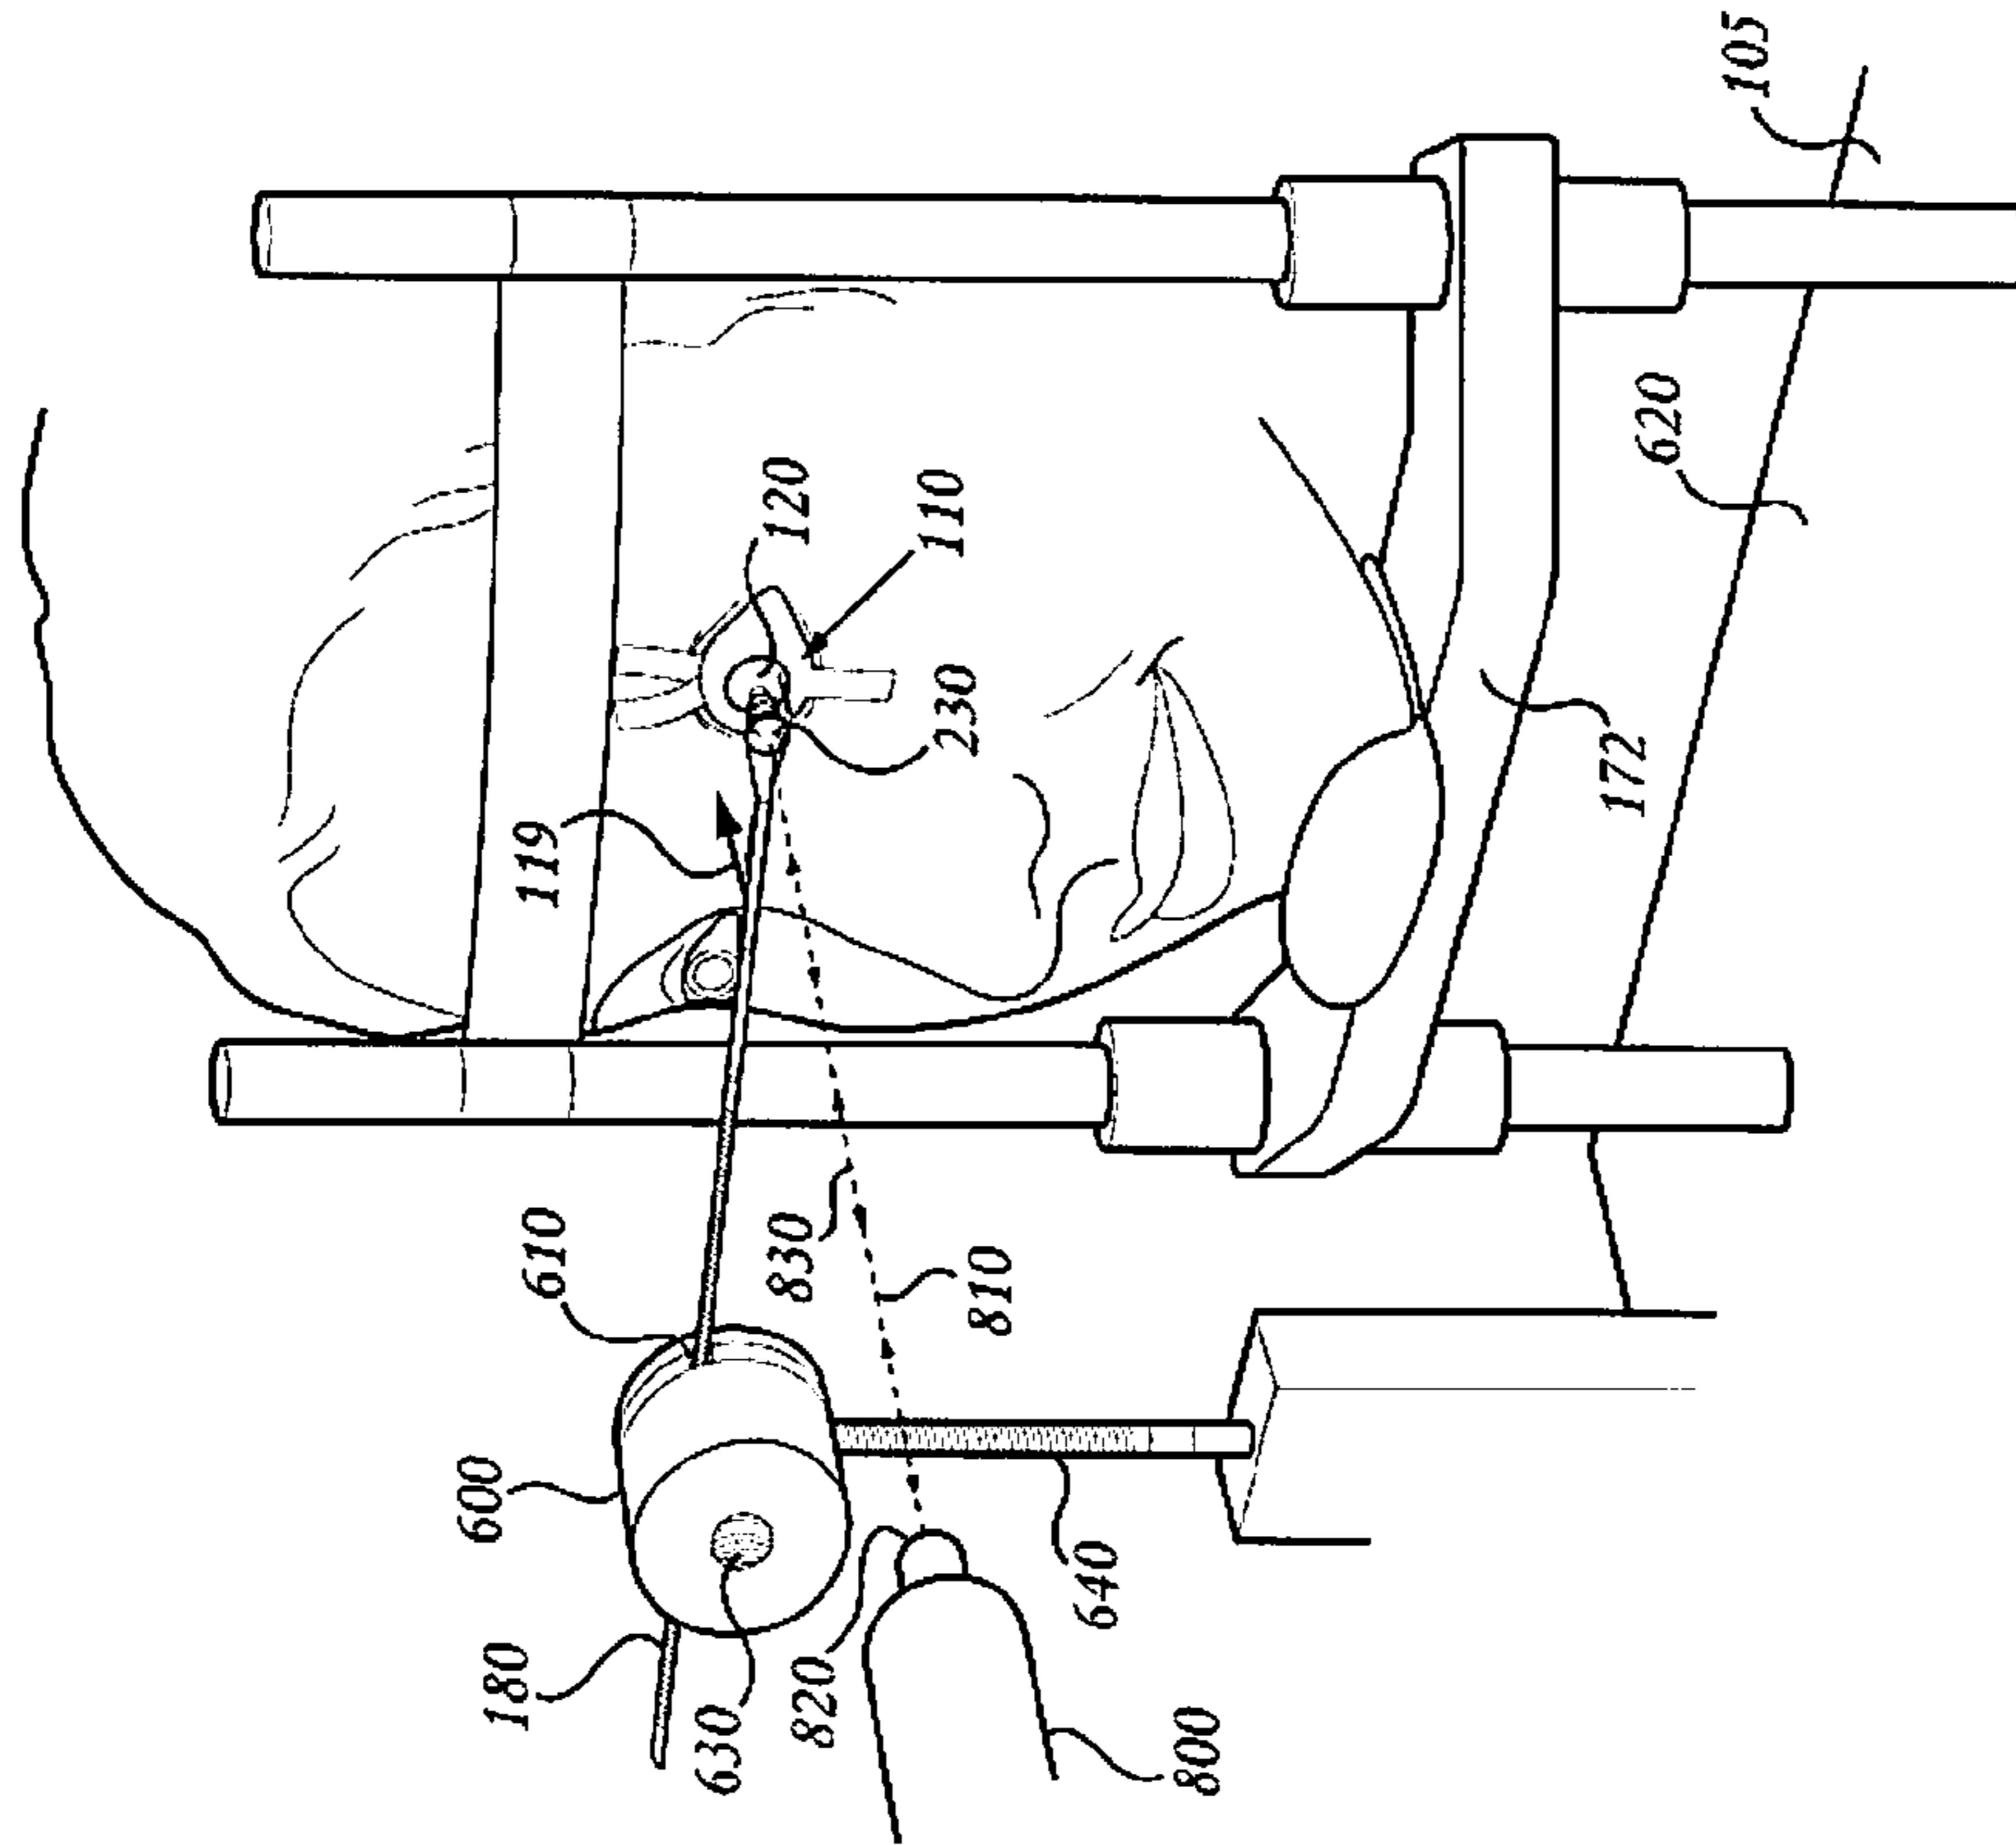


FIG. 8A

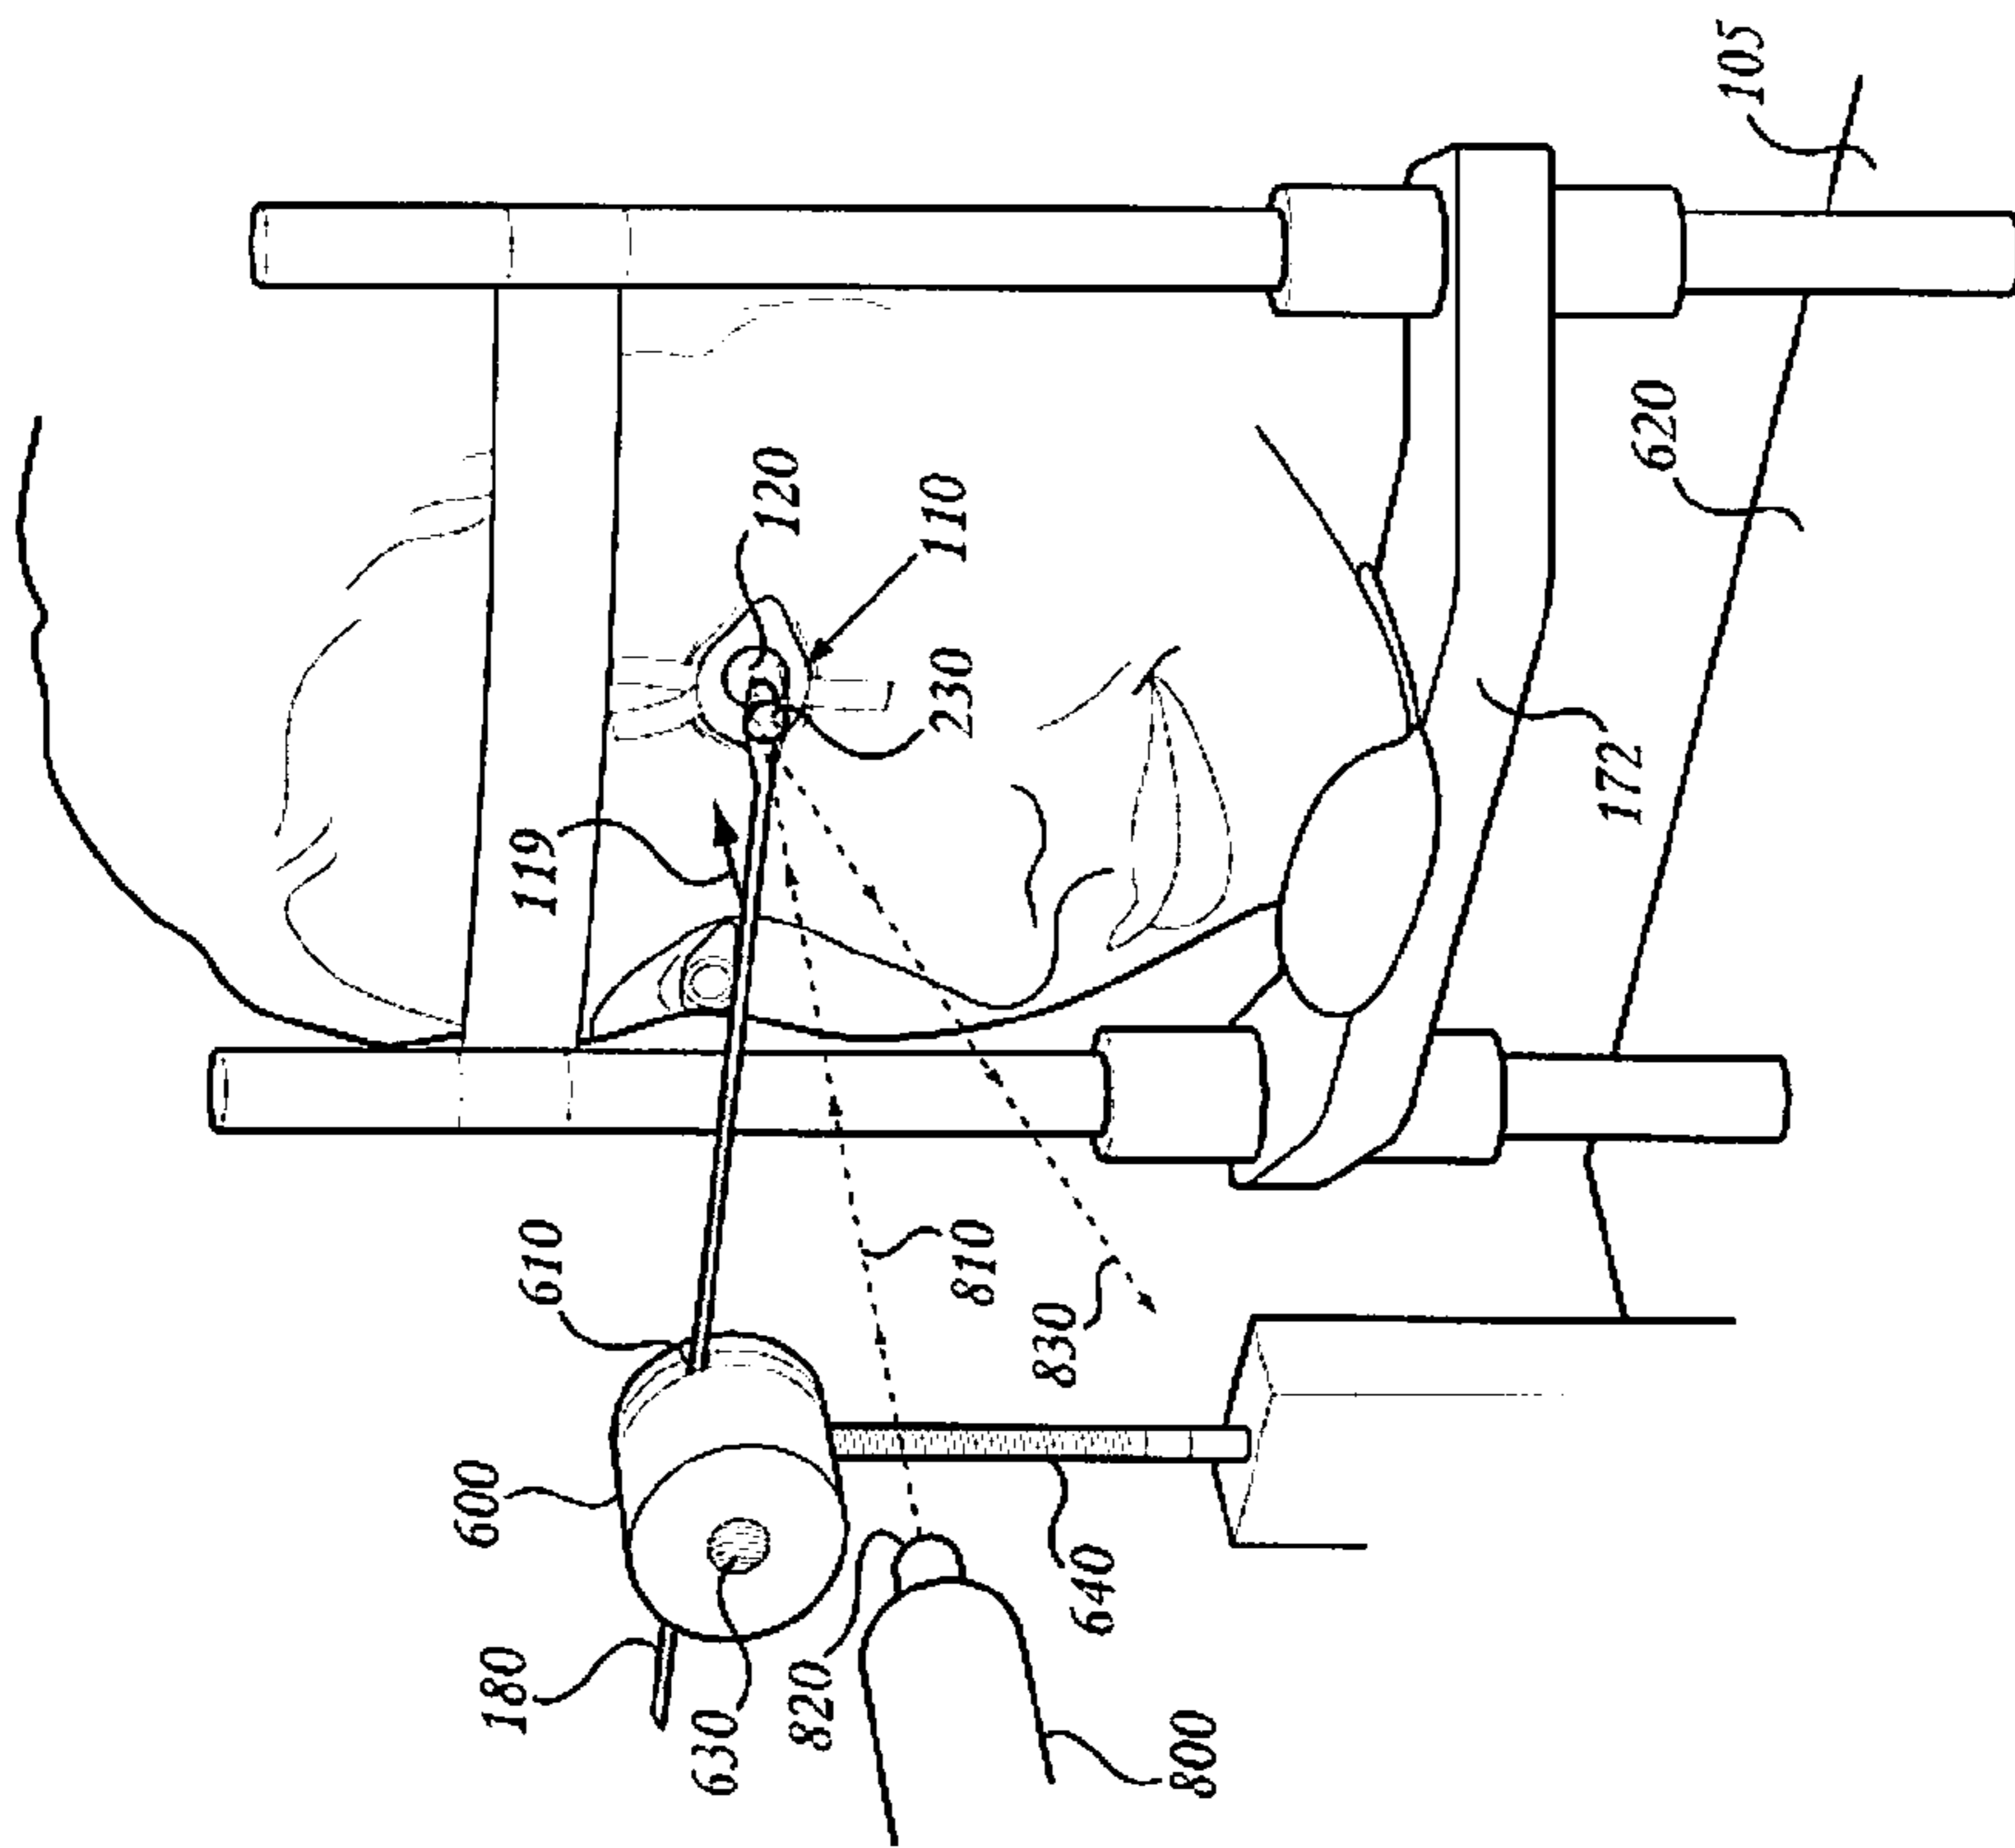


FIG. 8B

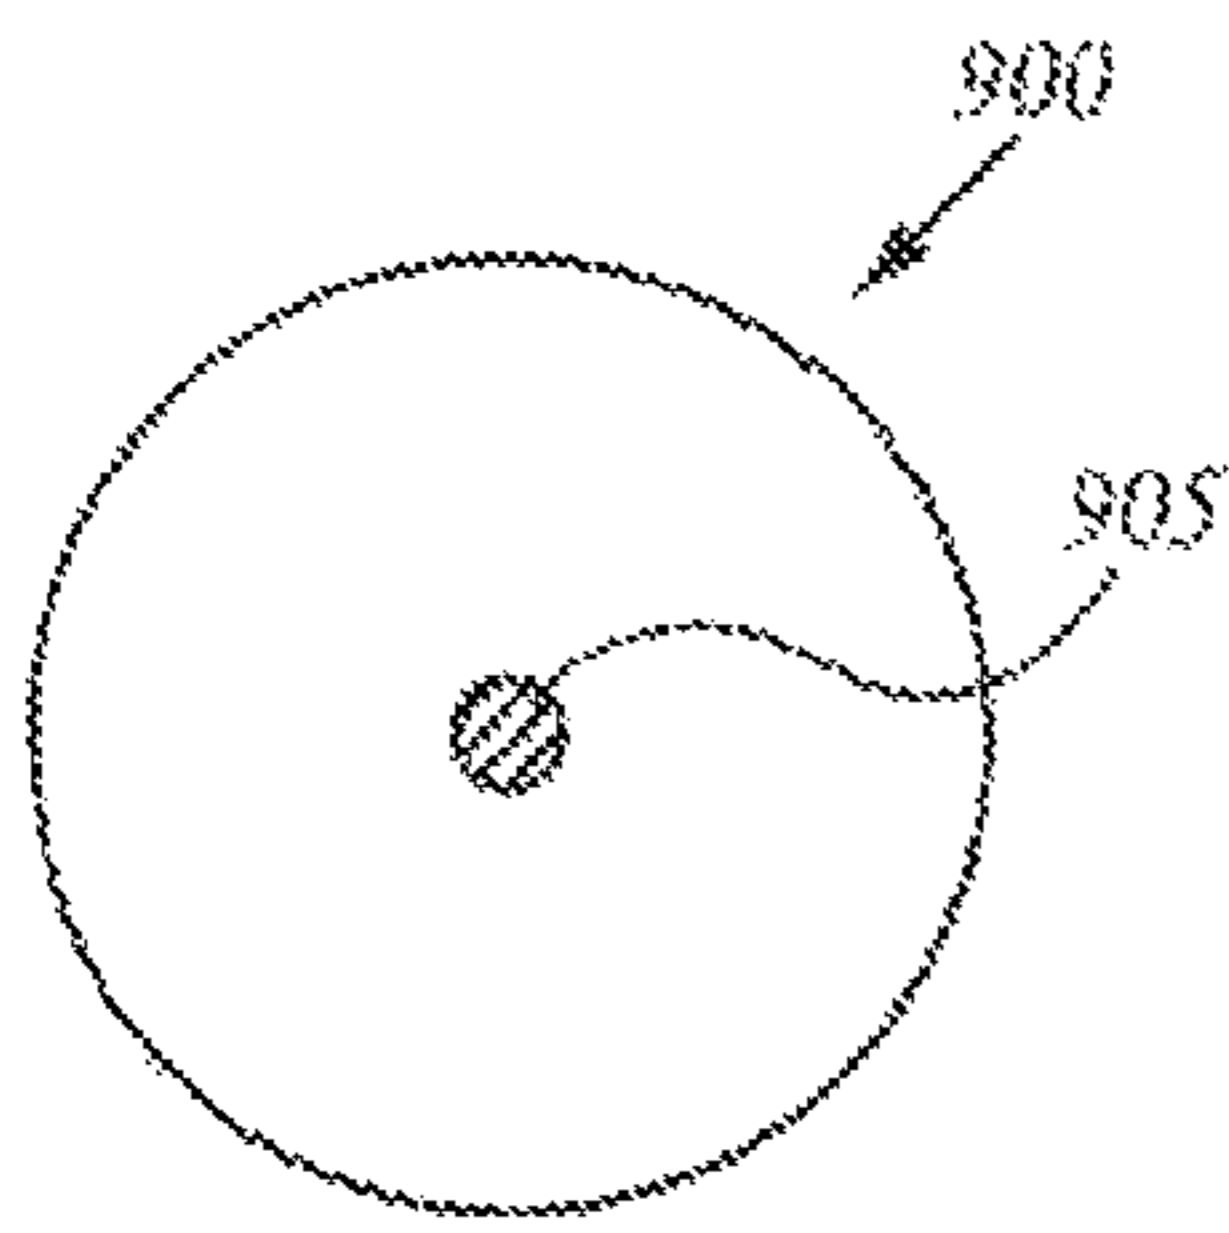


FIG. 9

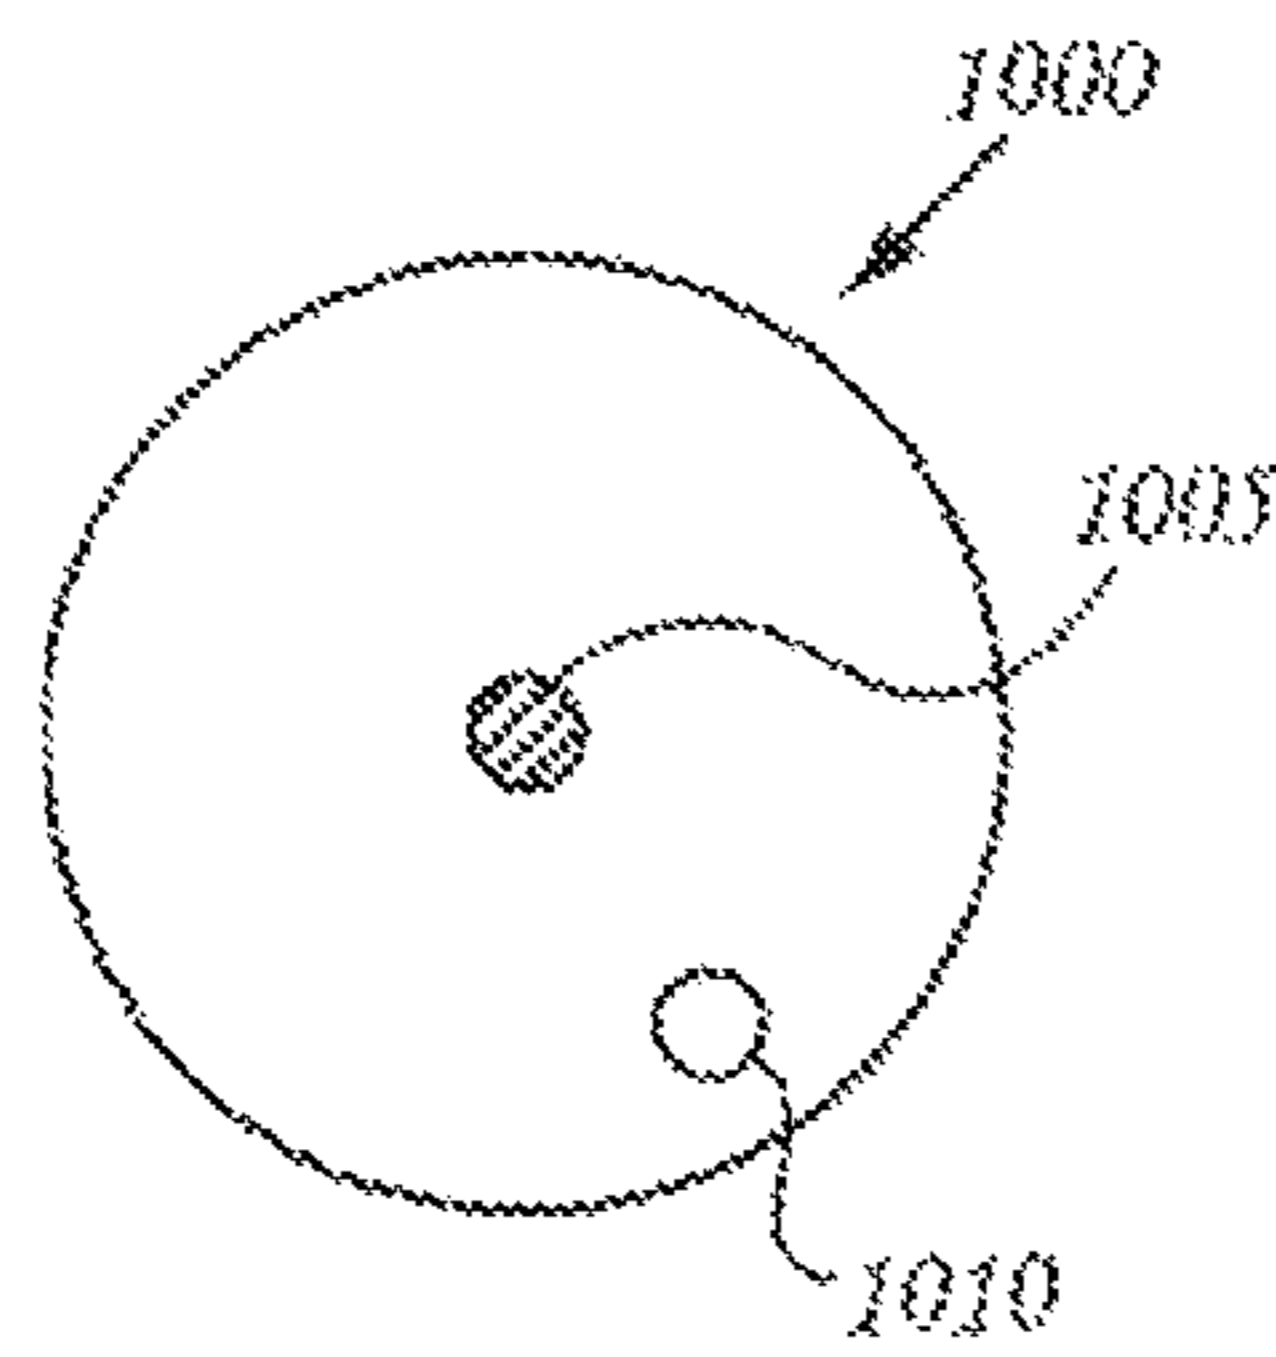


FIG. 10

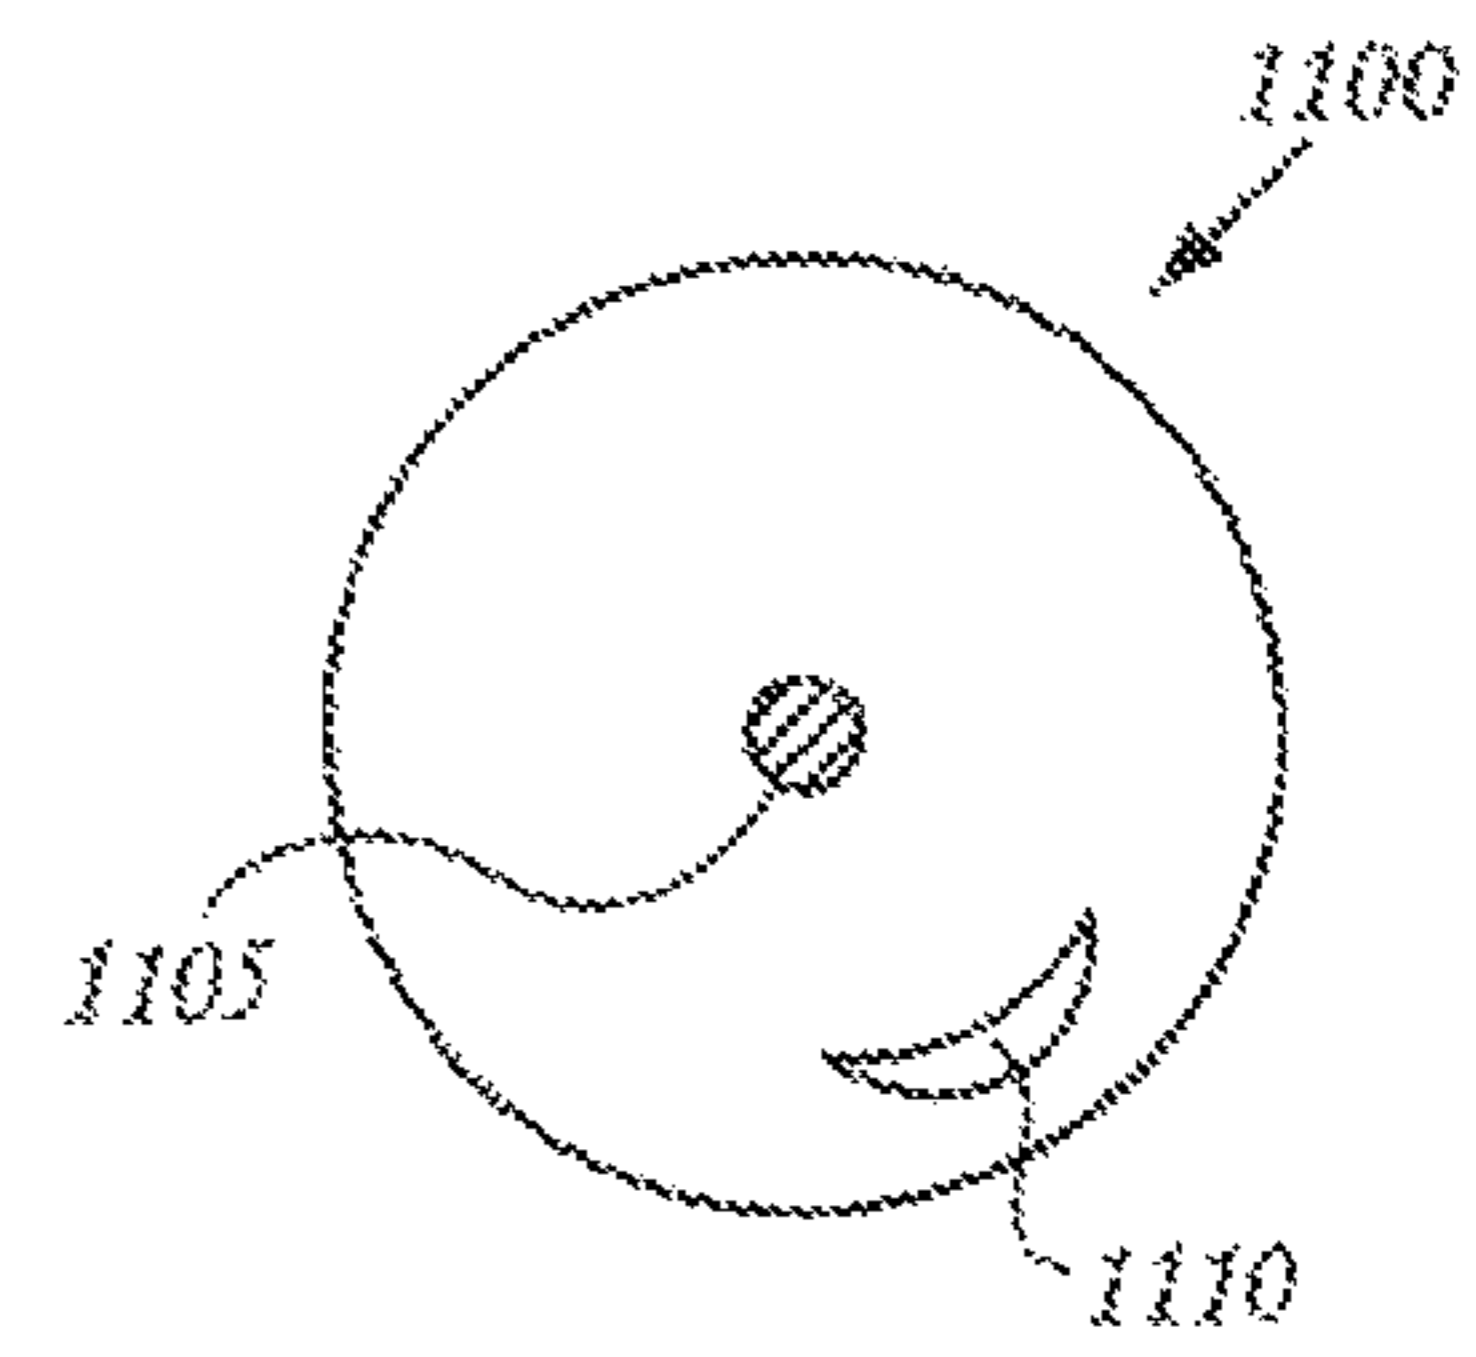


FIG. 11

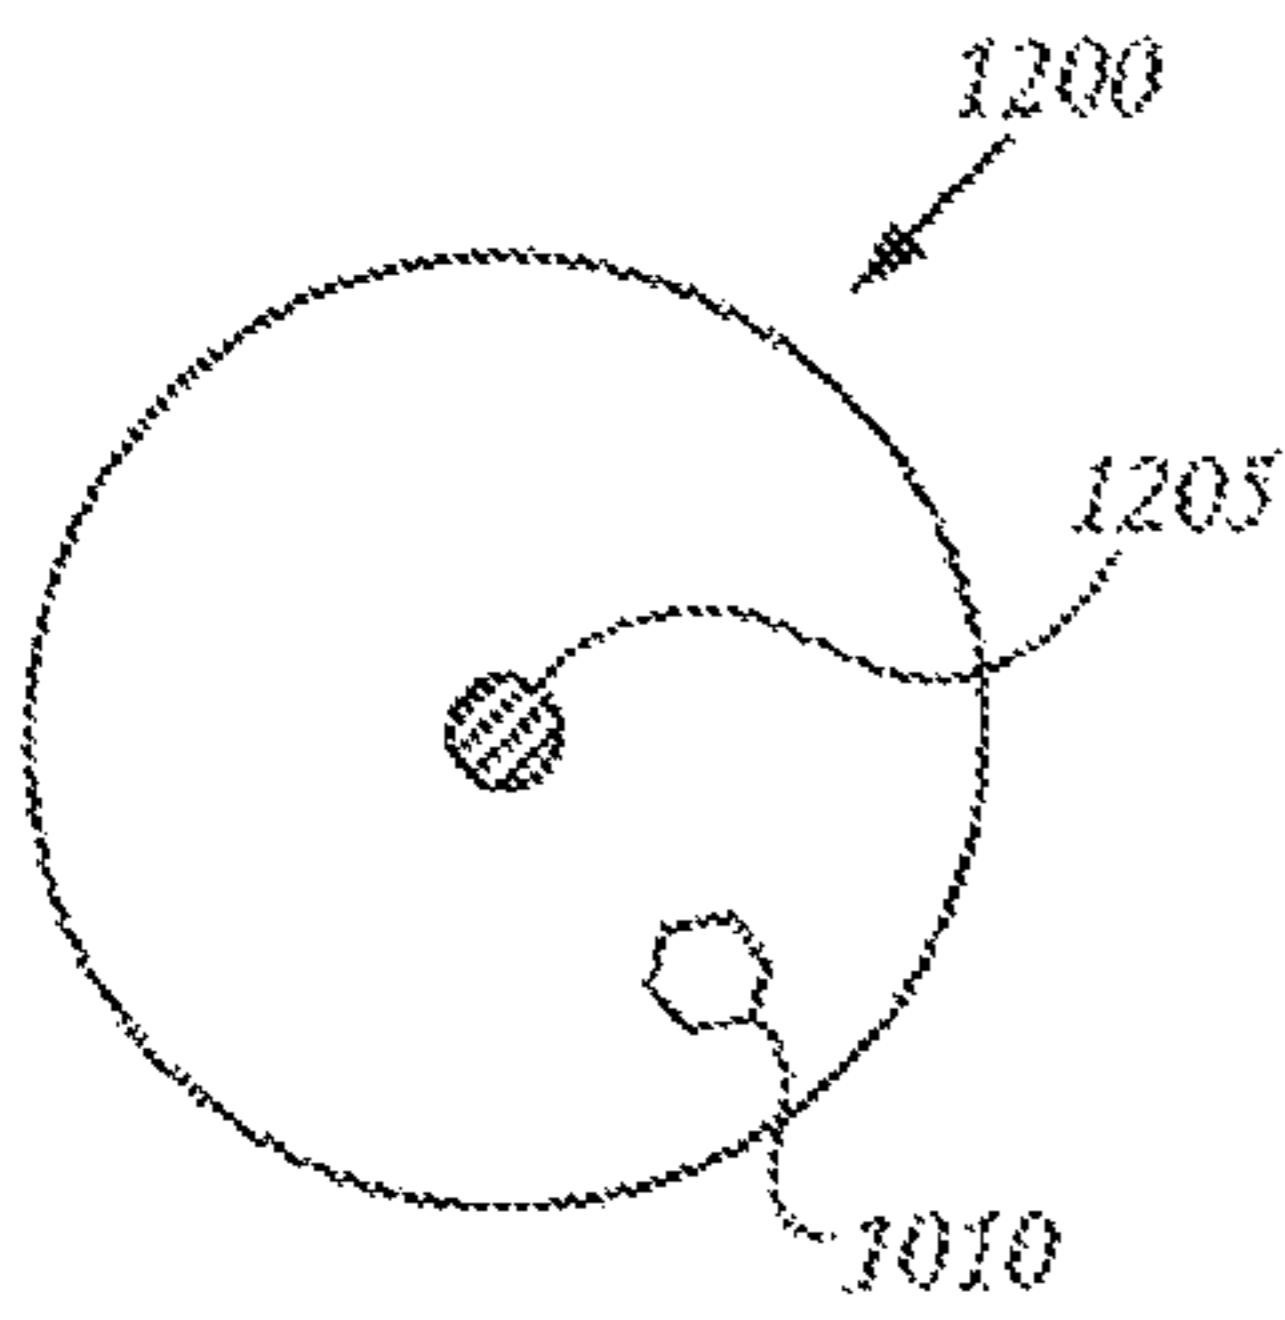


FIG. 12

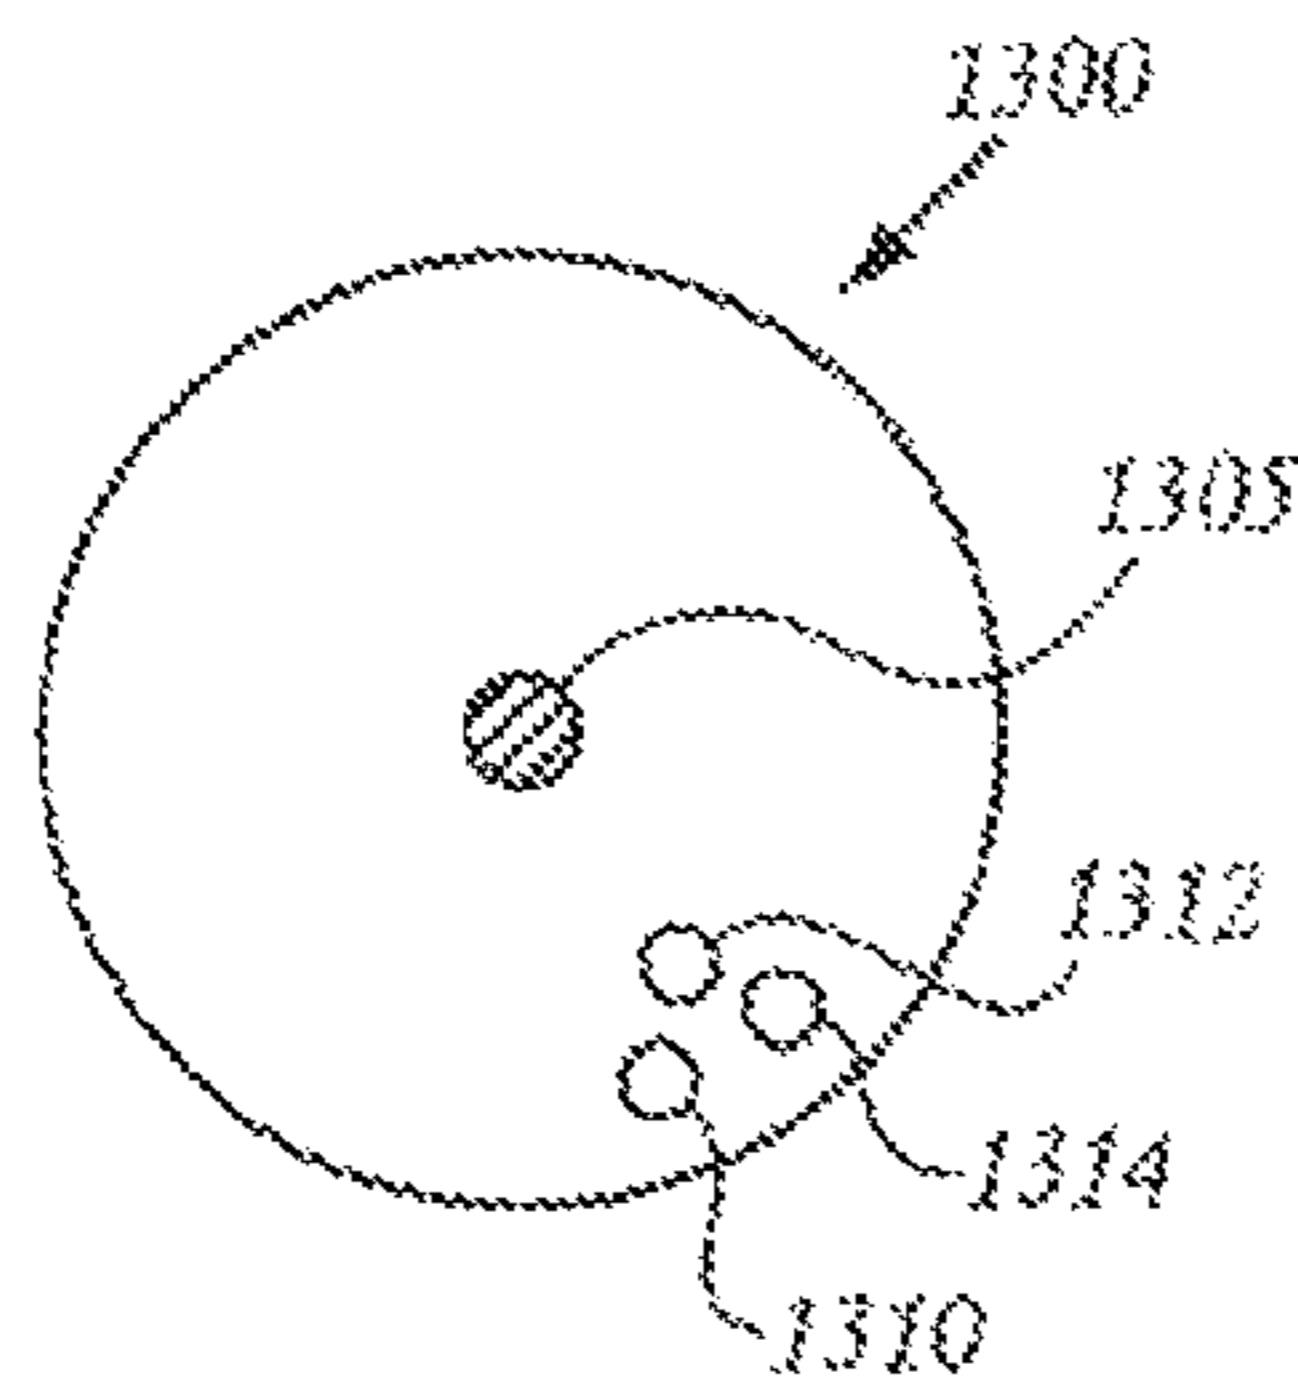


FIG. 13

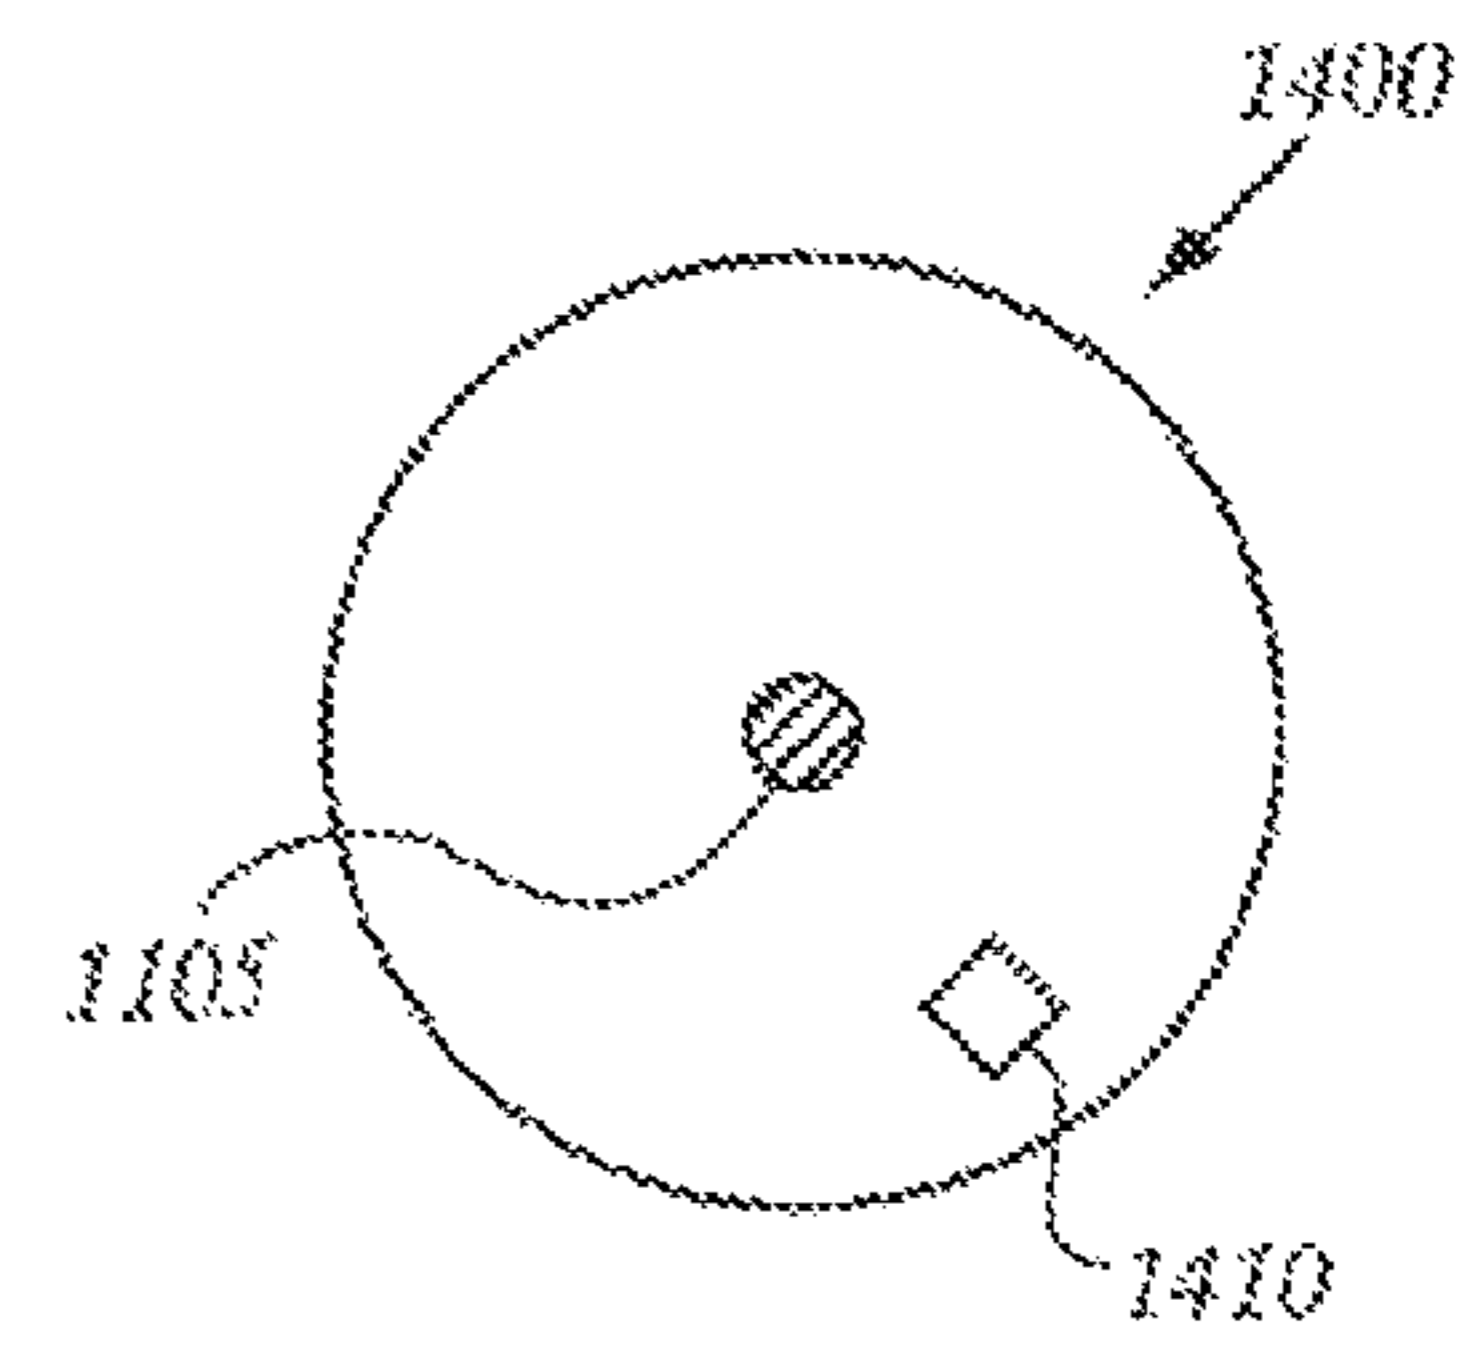


FIG. 14

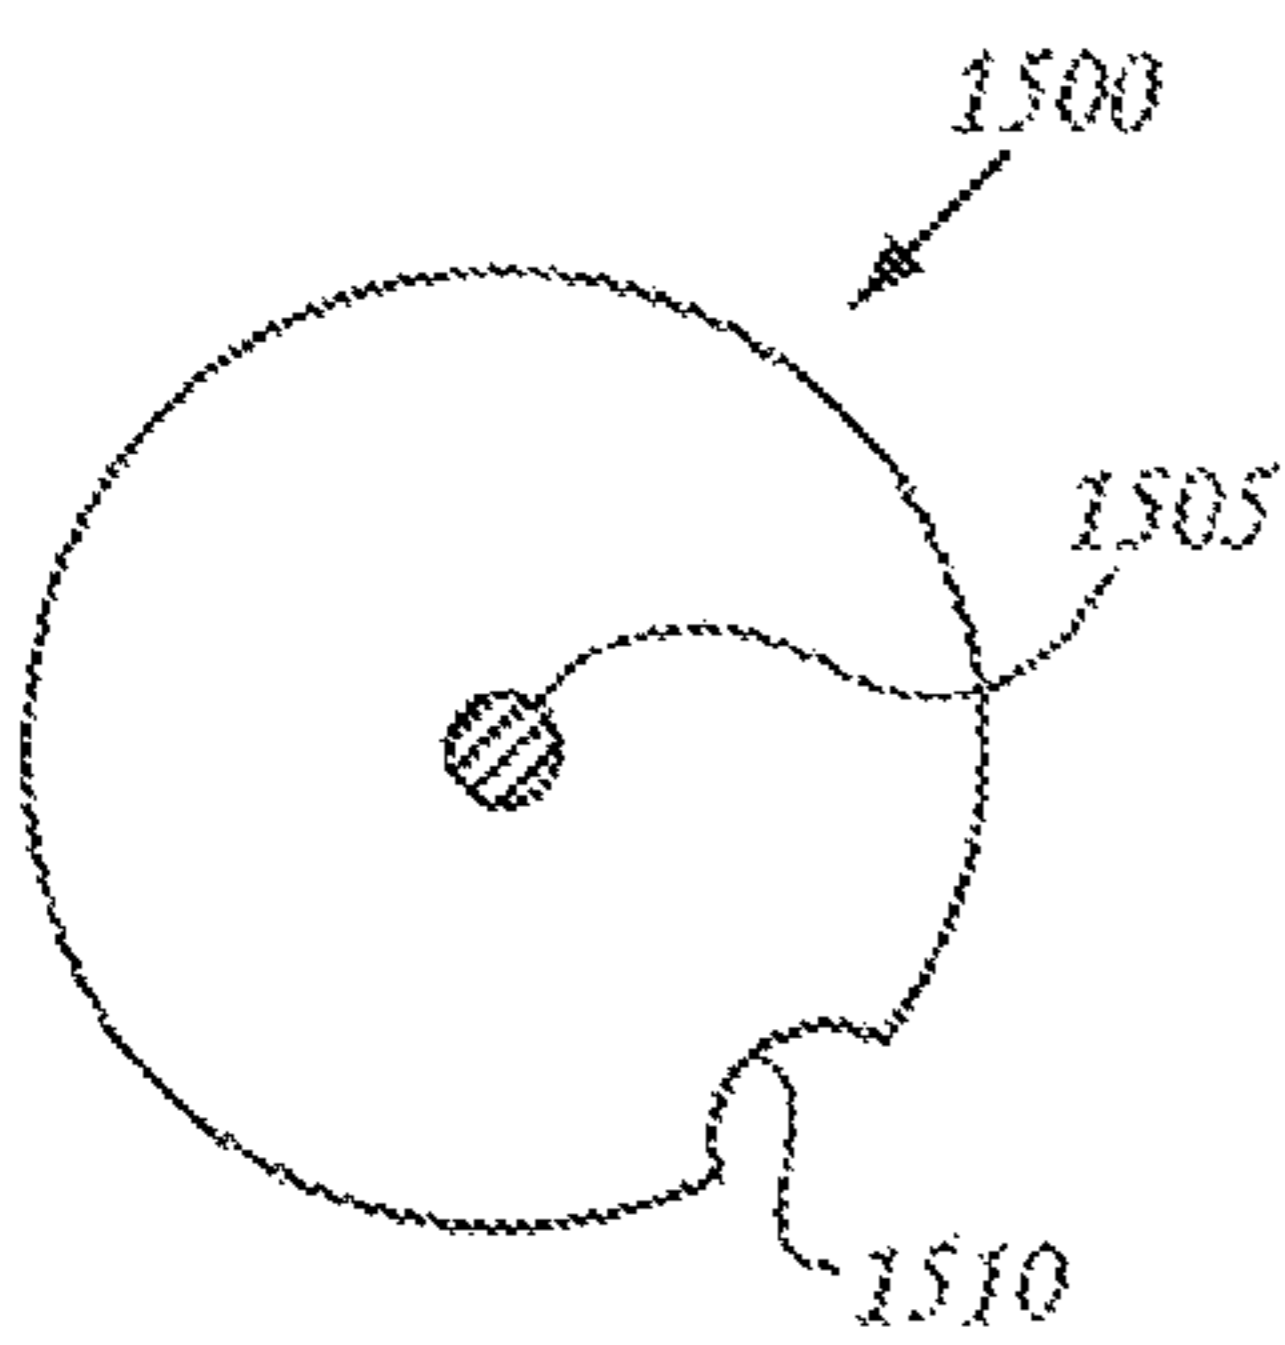


FIG. 15

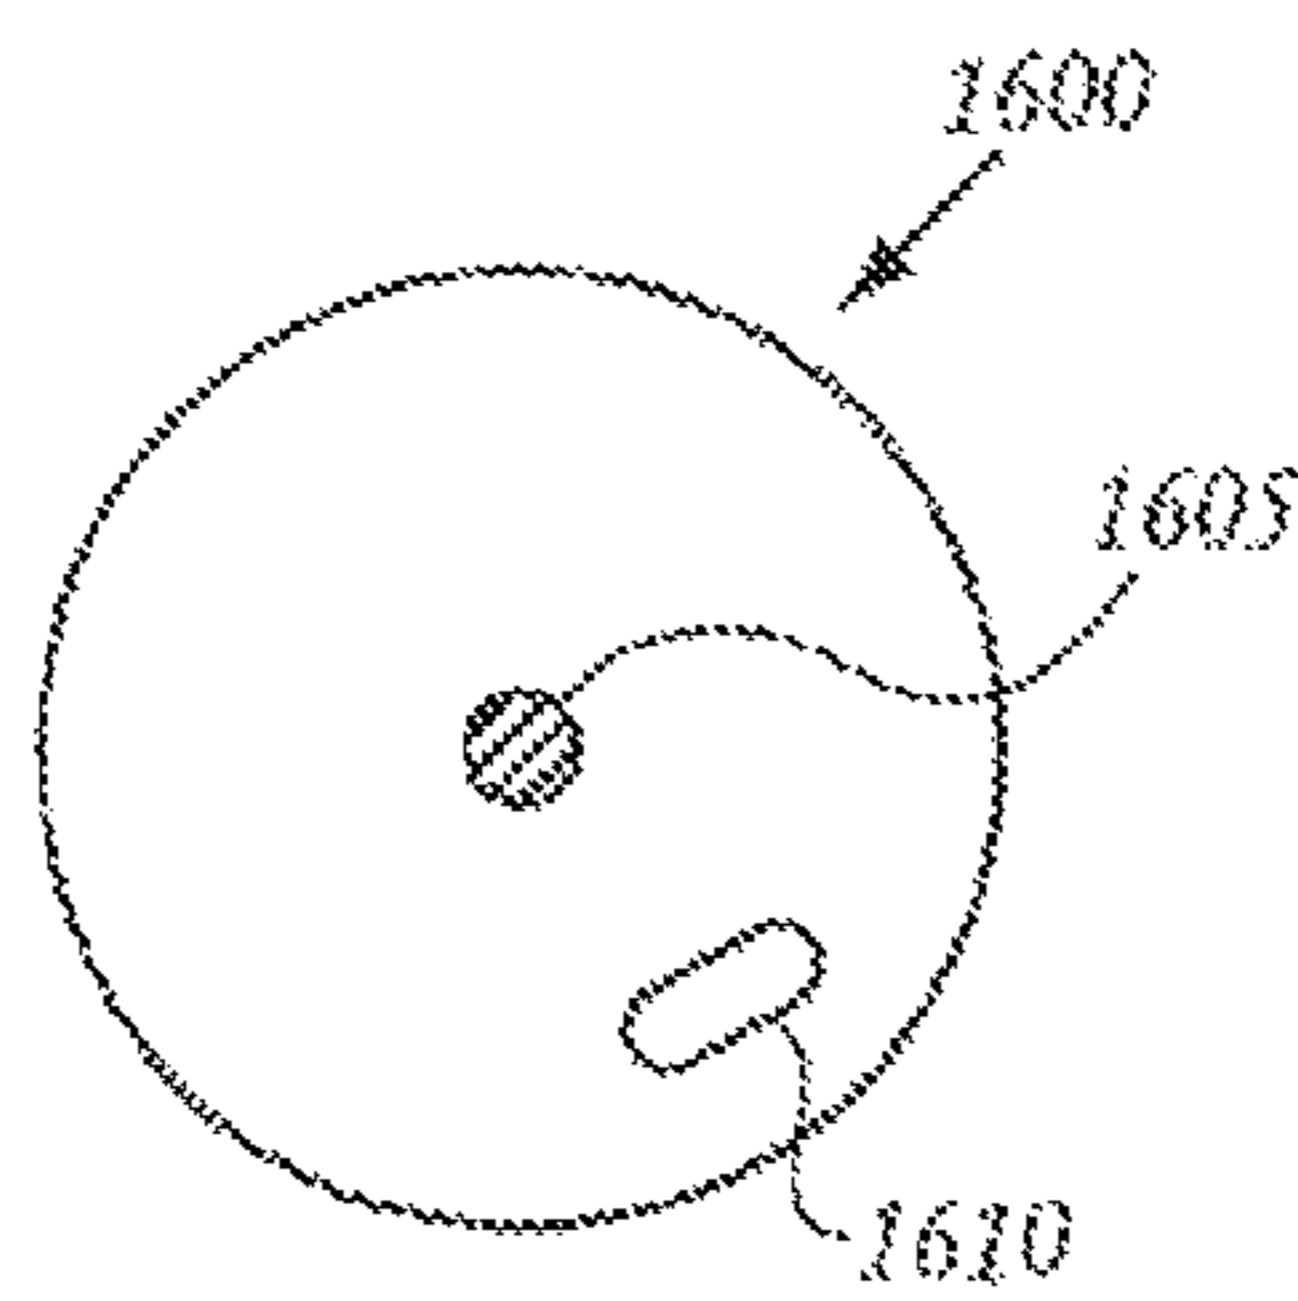


FIG. 16

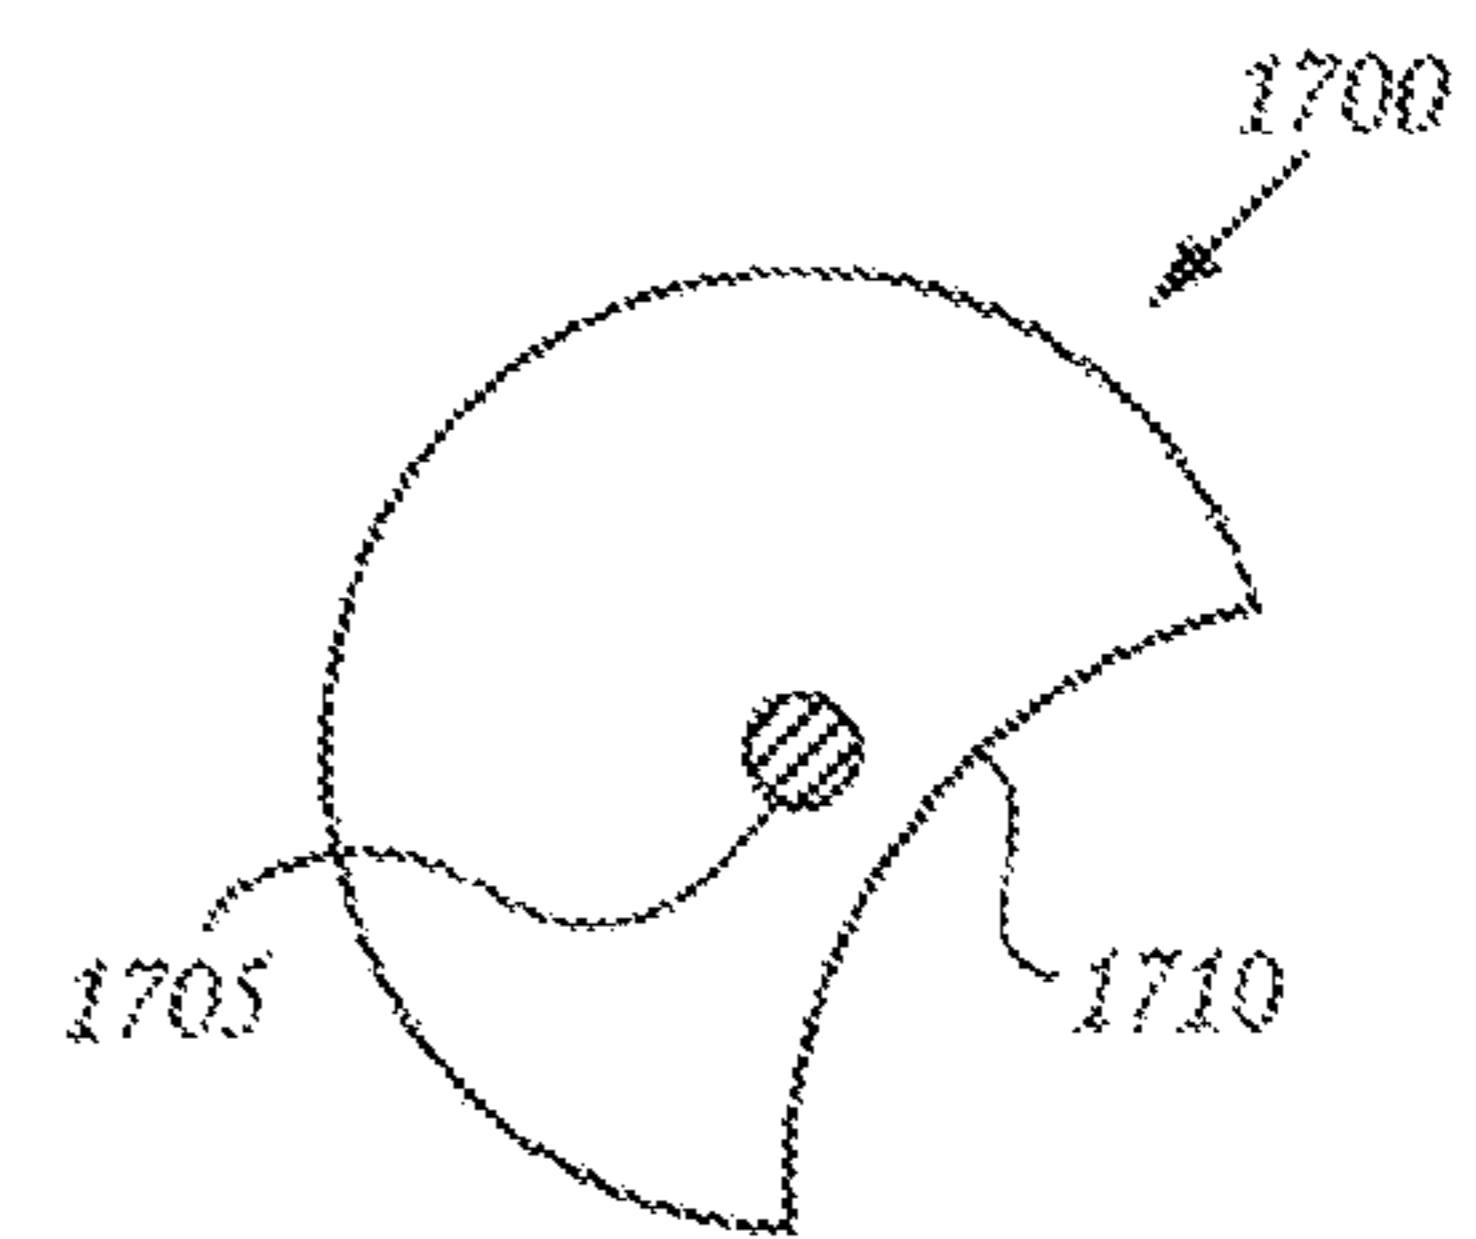


FIG. 17

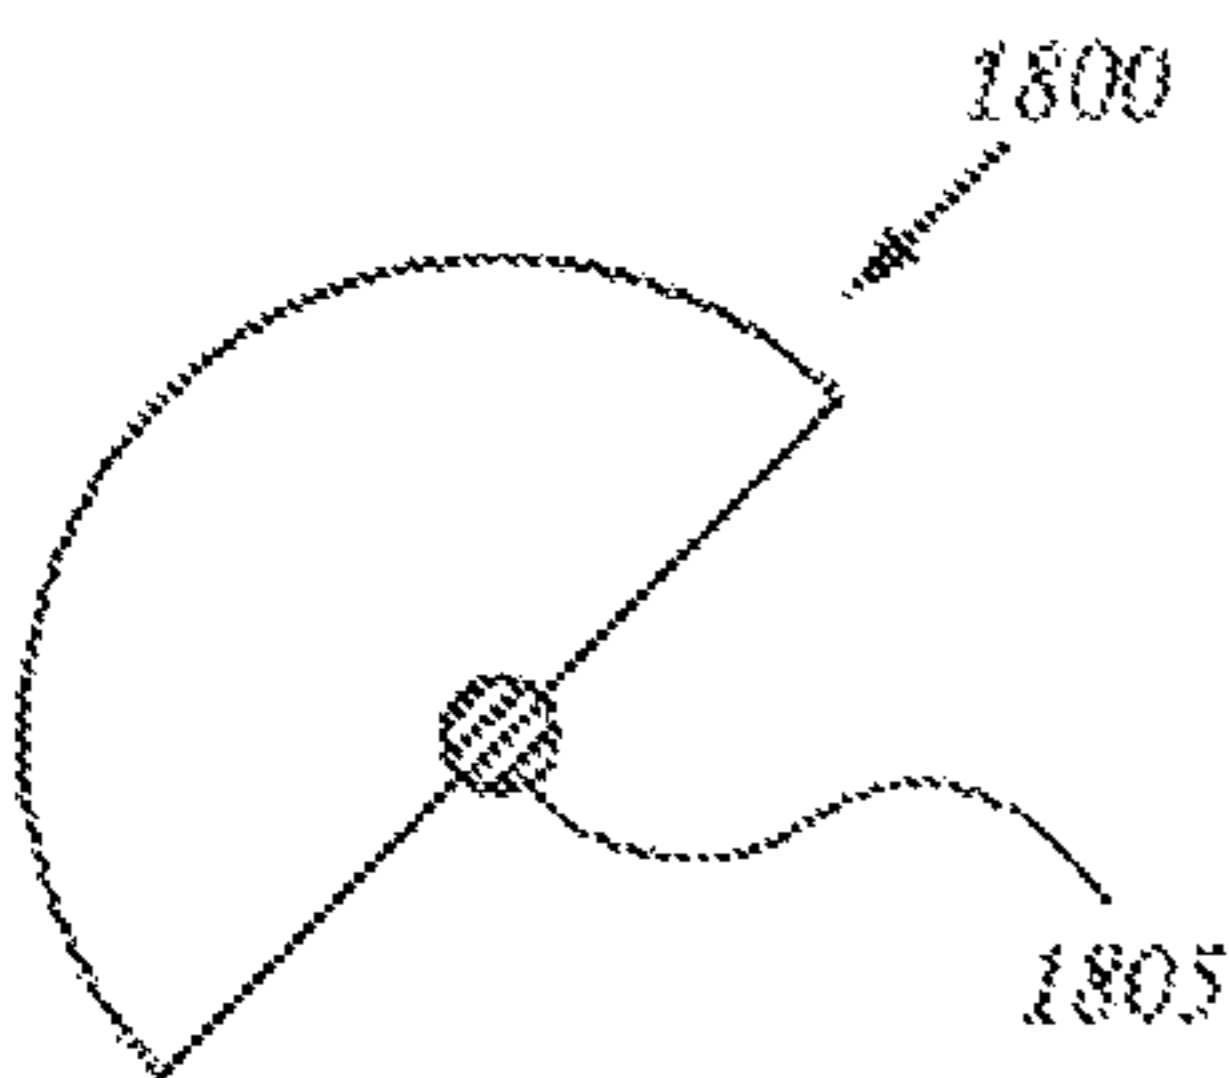


FIG. 18A

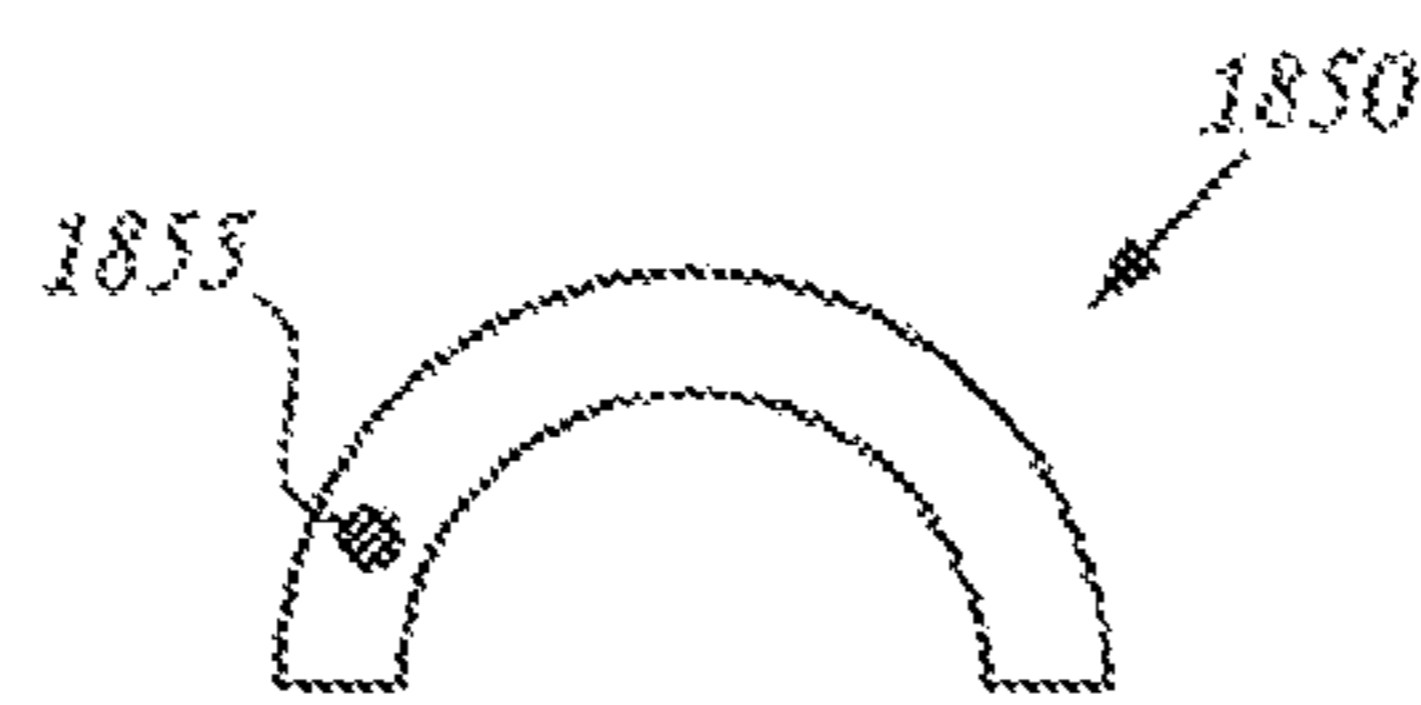


FIG. 18B



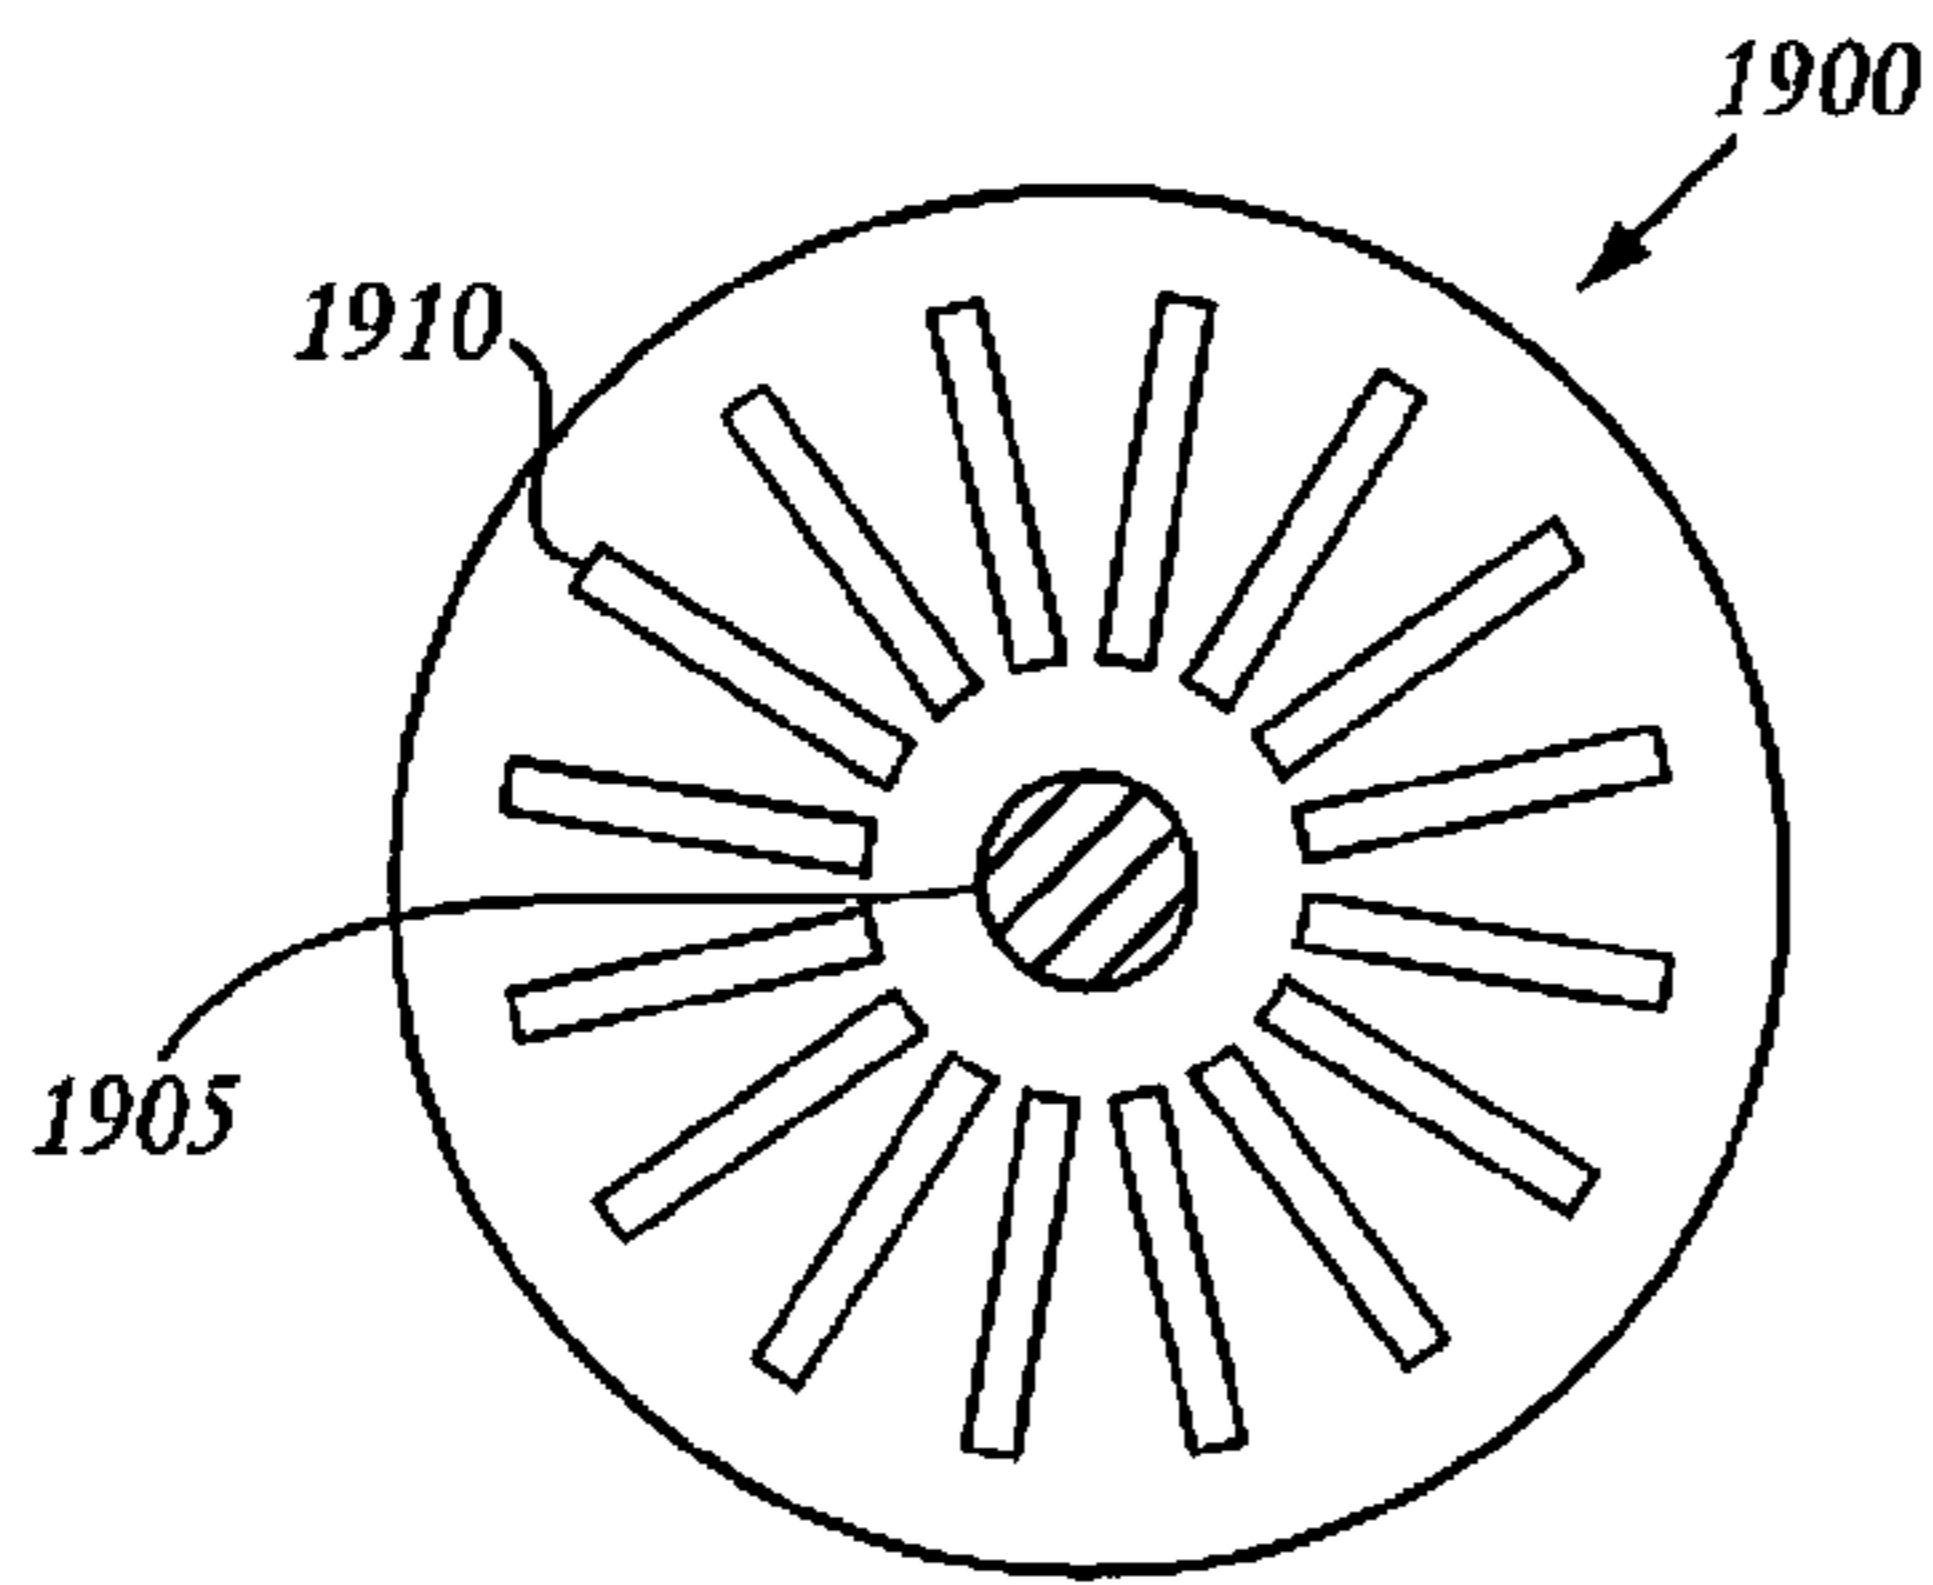


FIG. 19

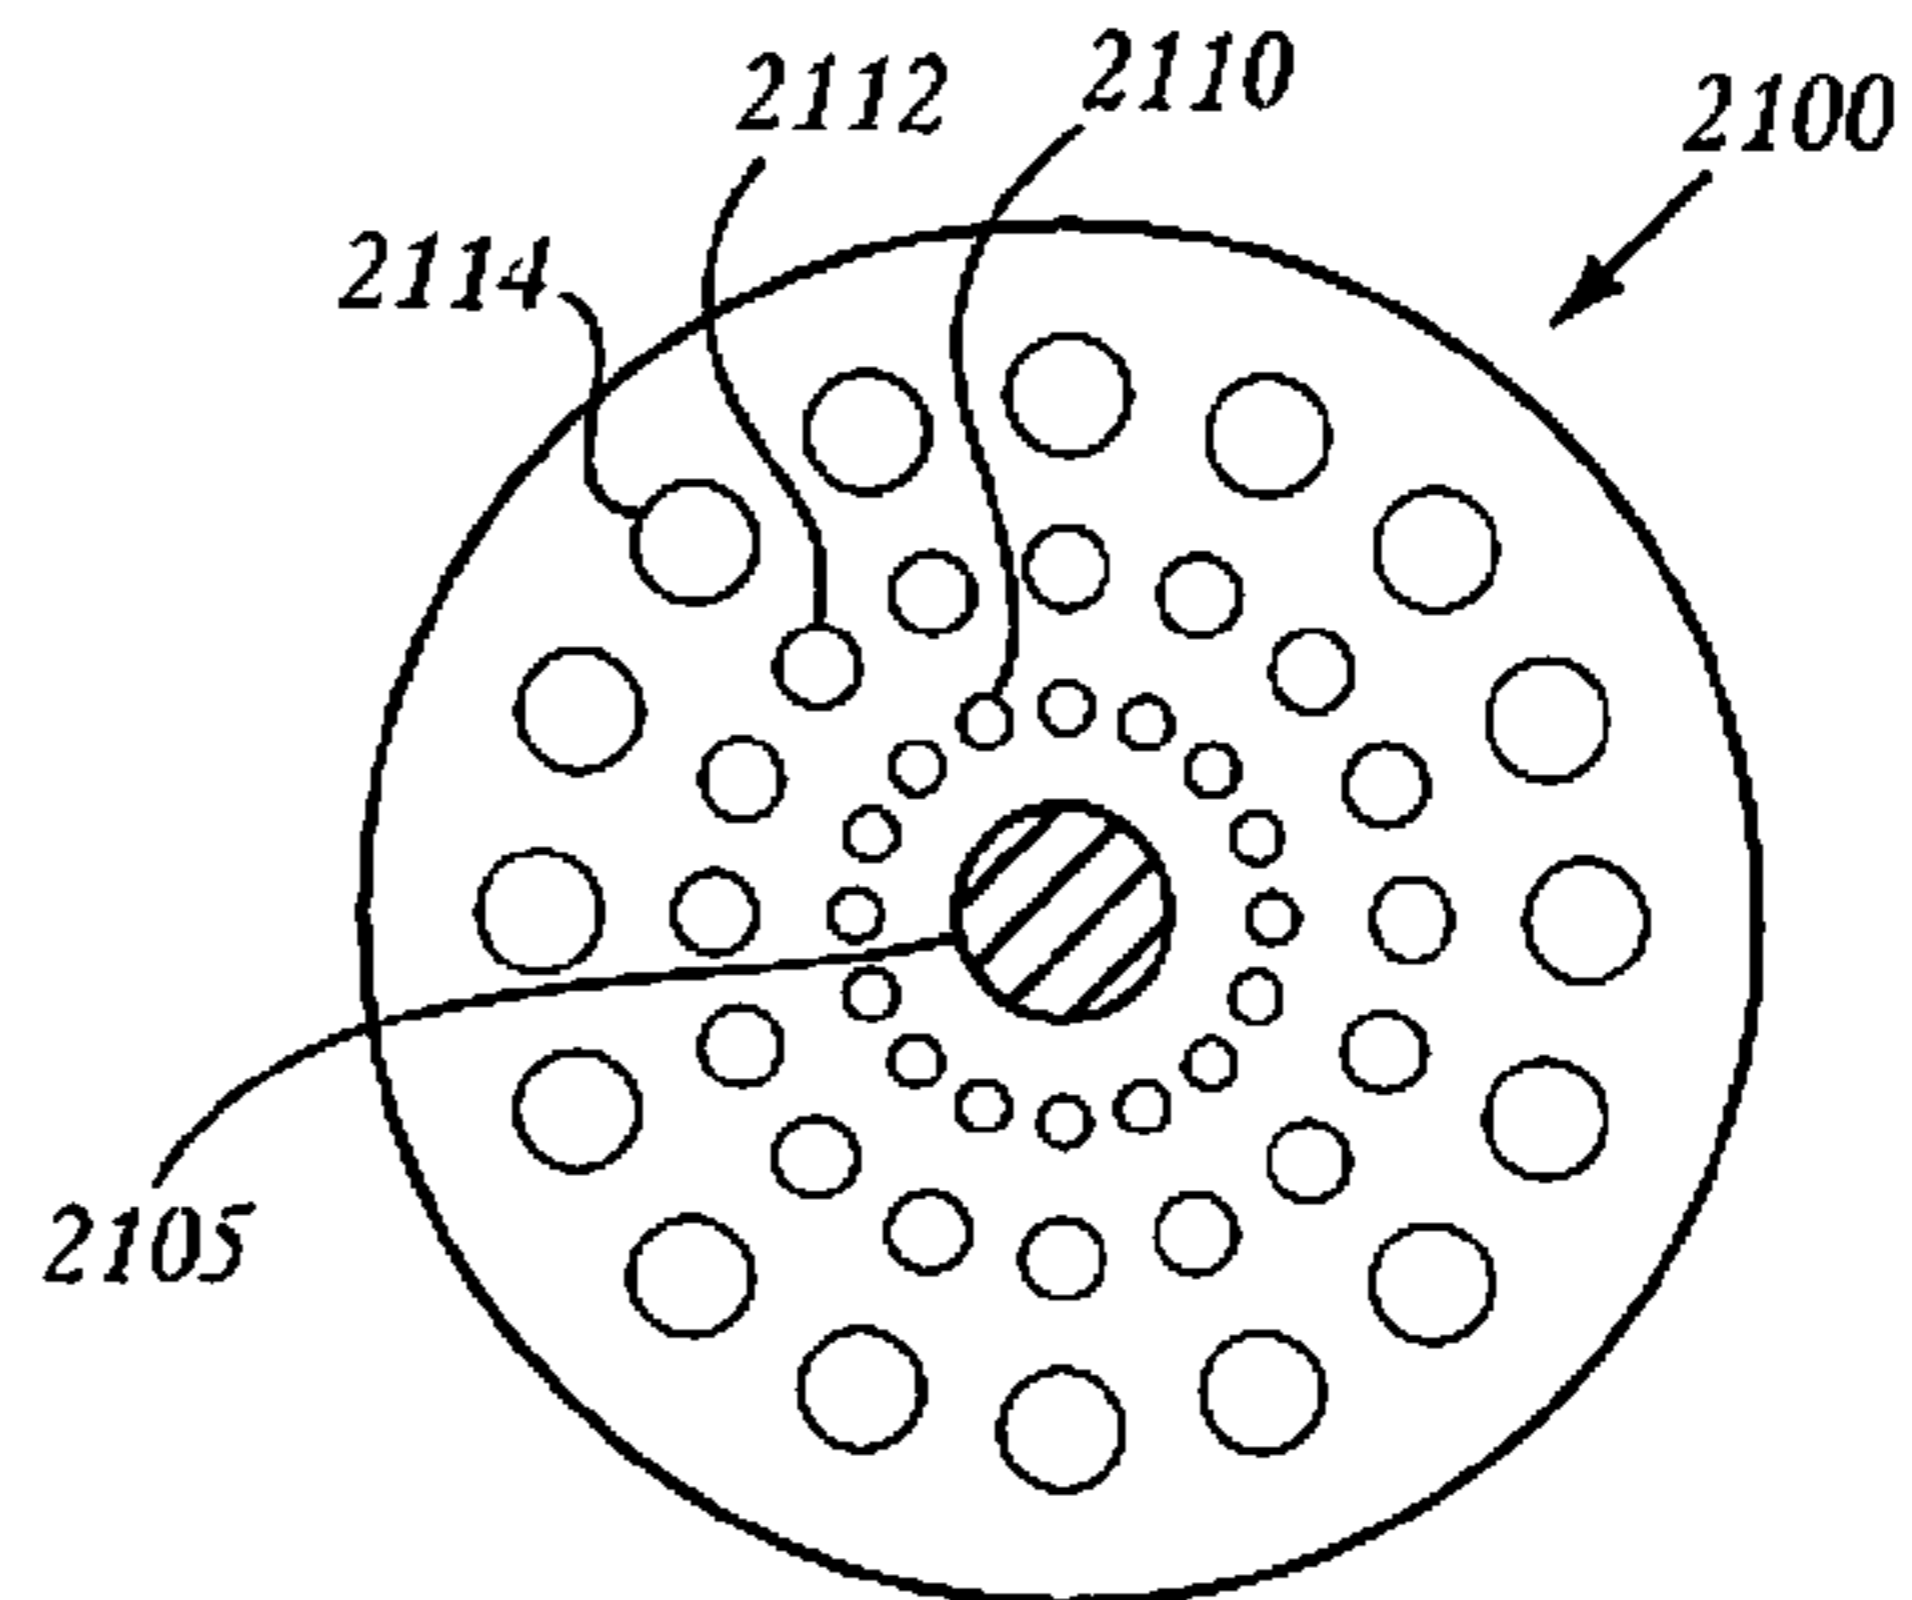


FIG. 21

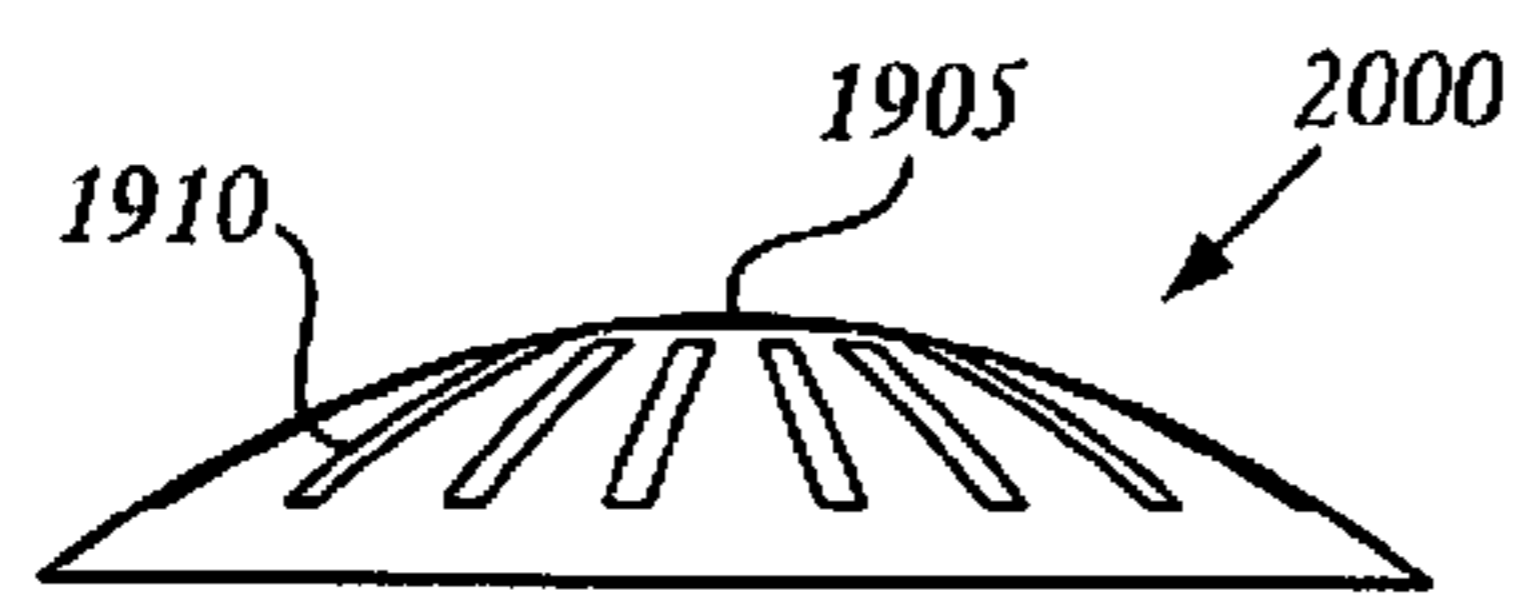


FIG. 20

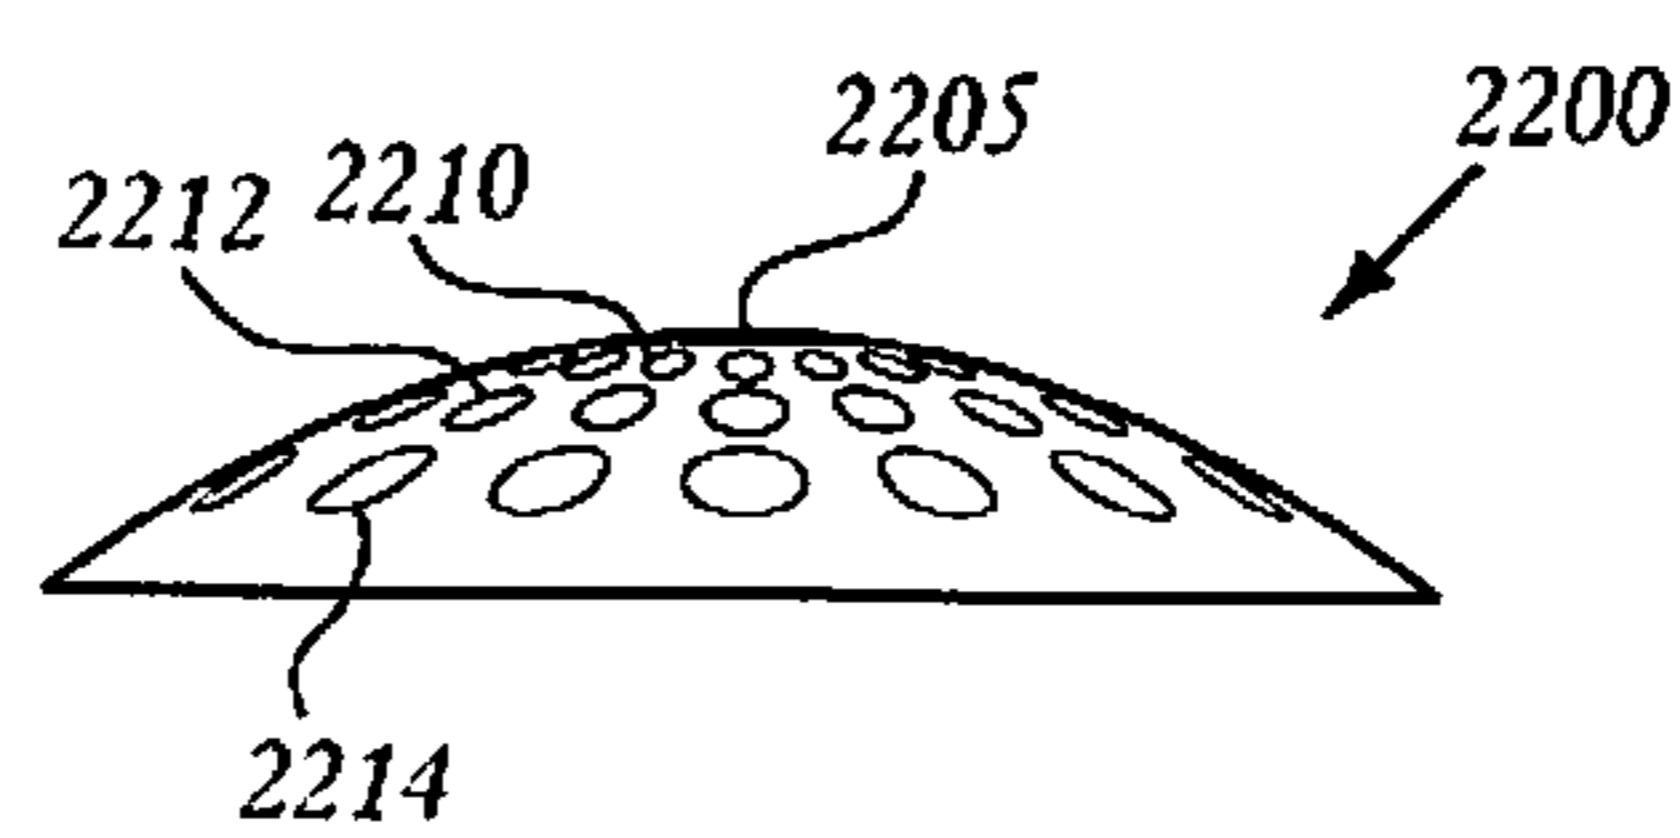


FIG. 22

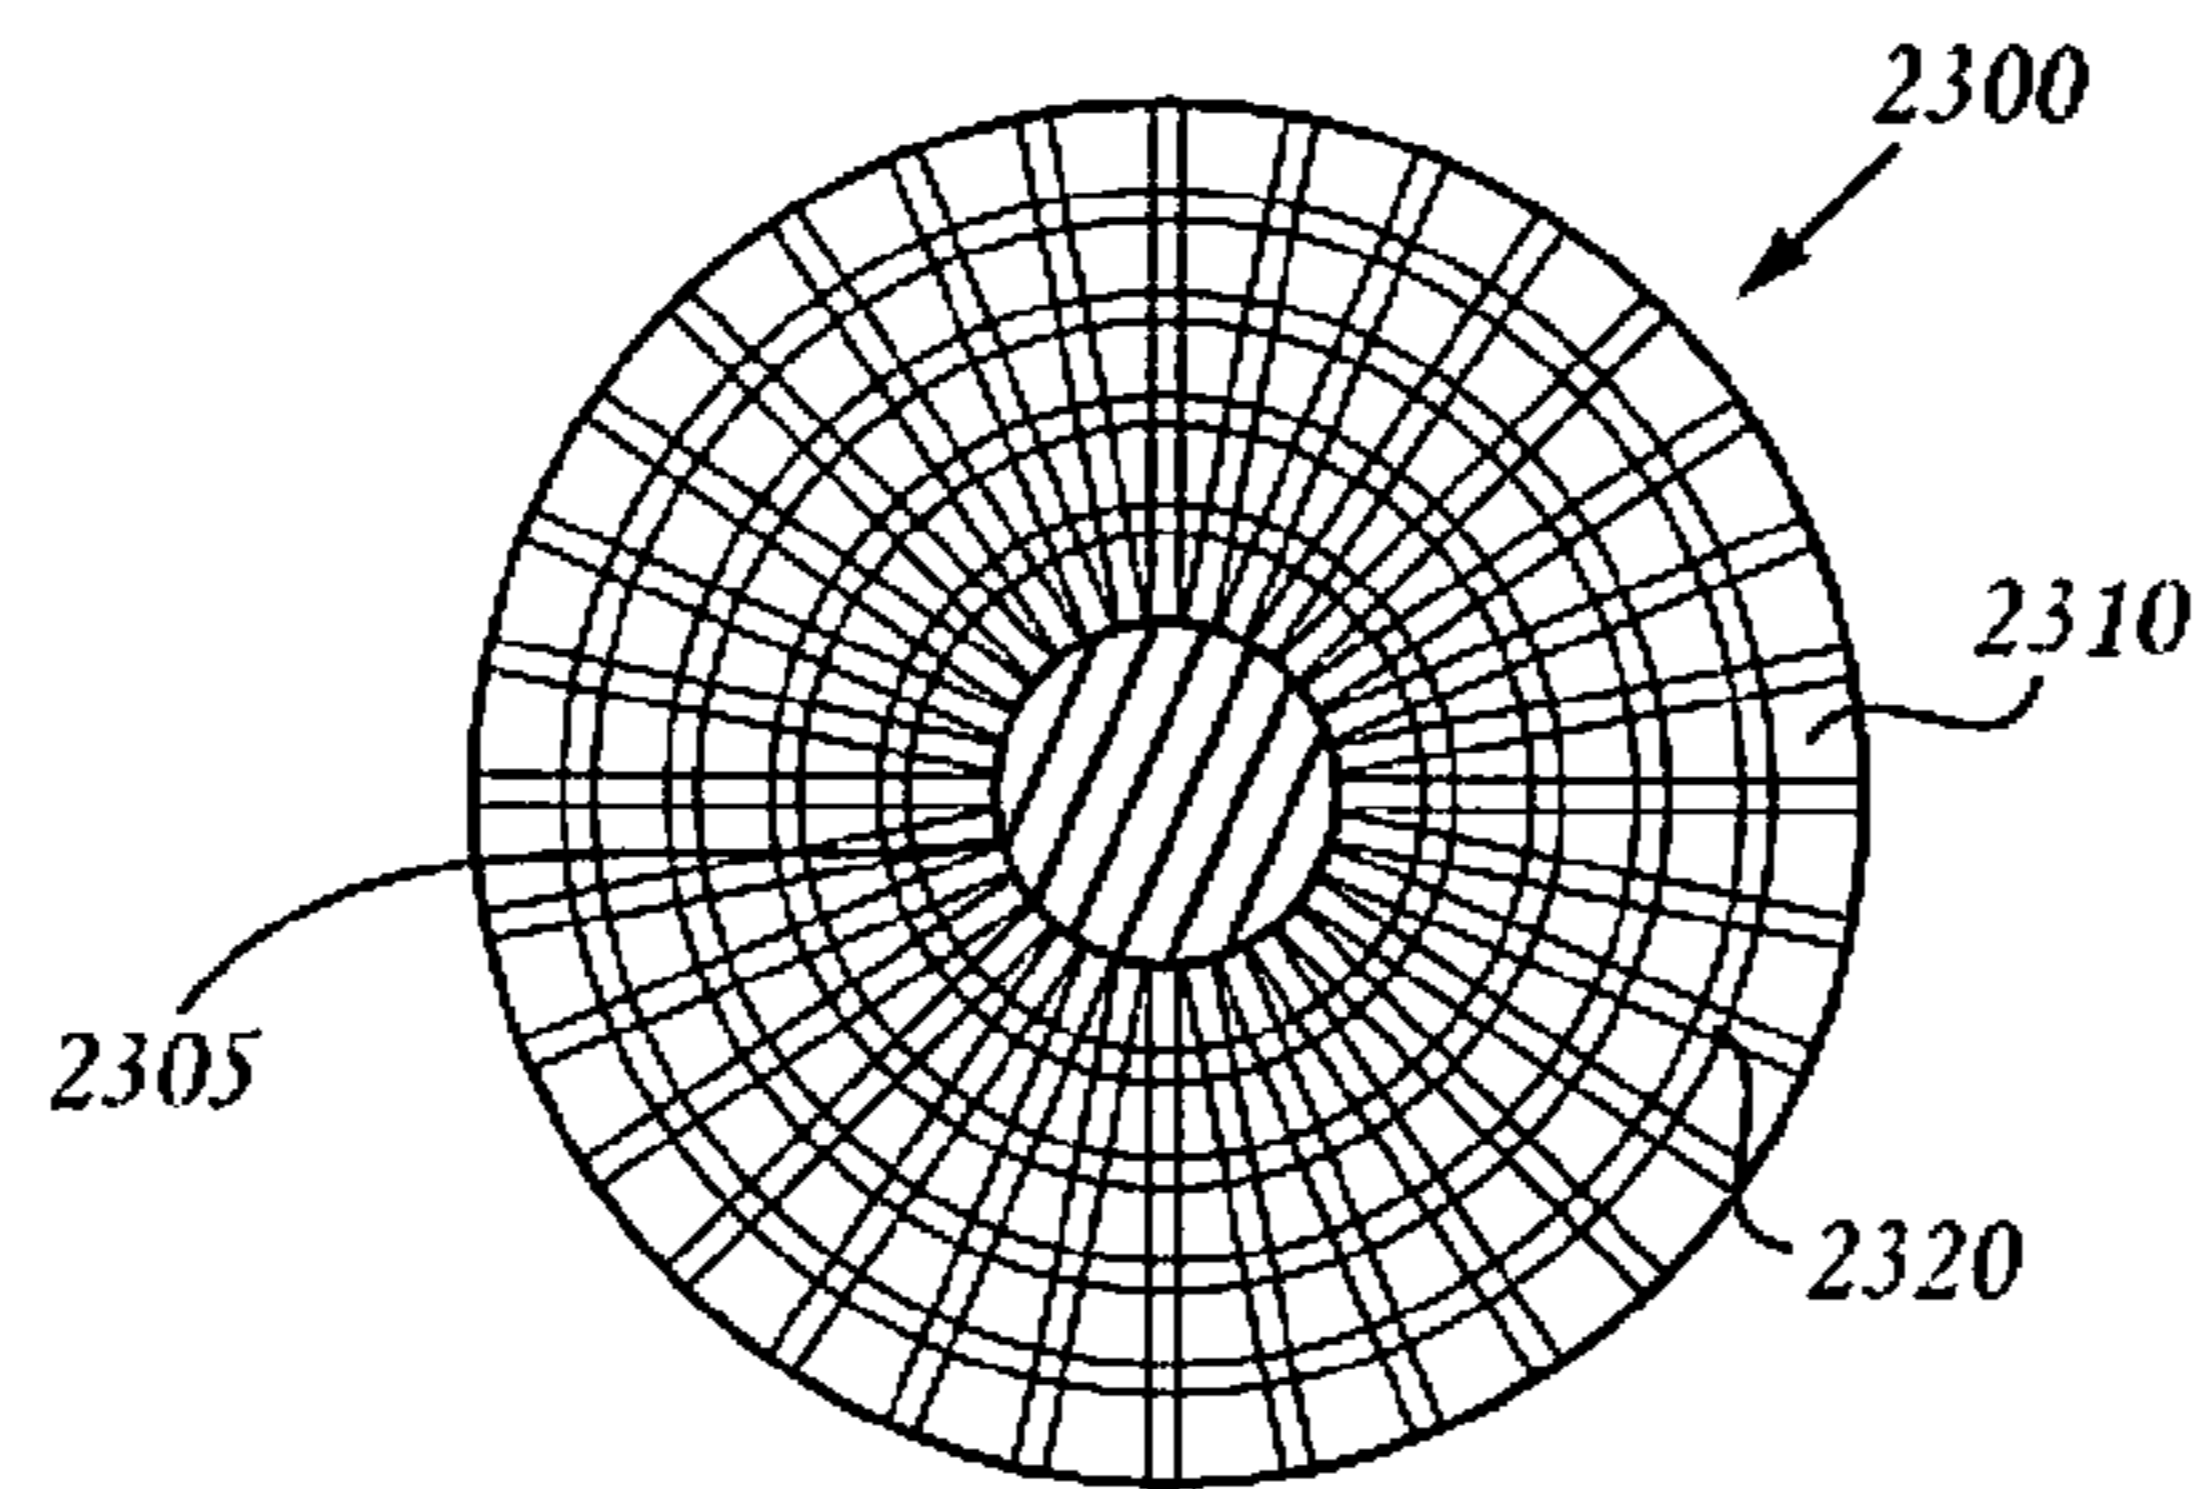


FIG. 23

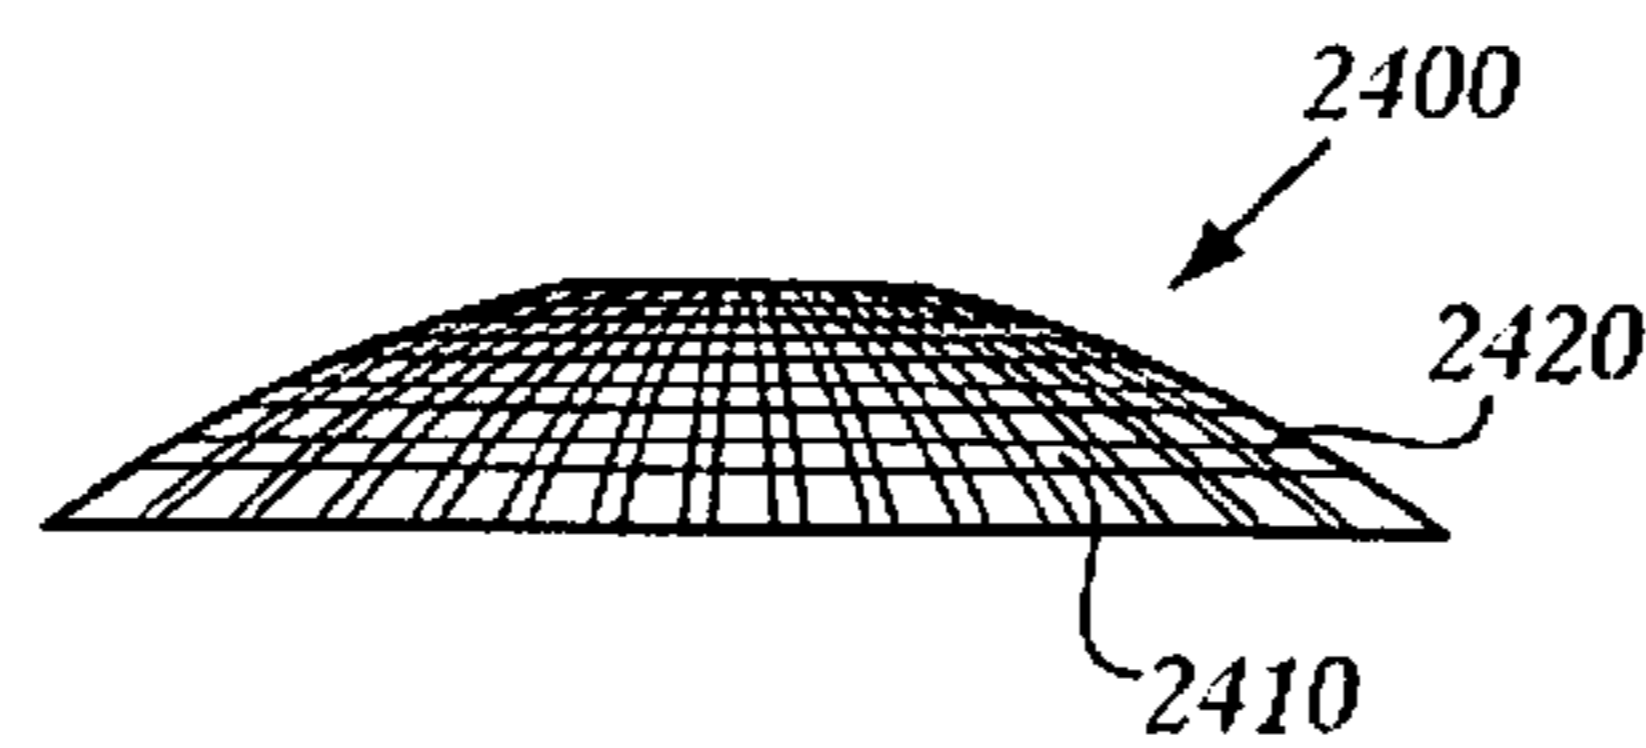


FIG. 24

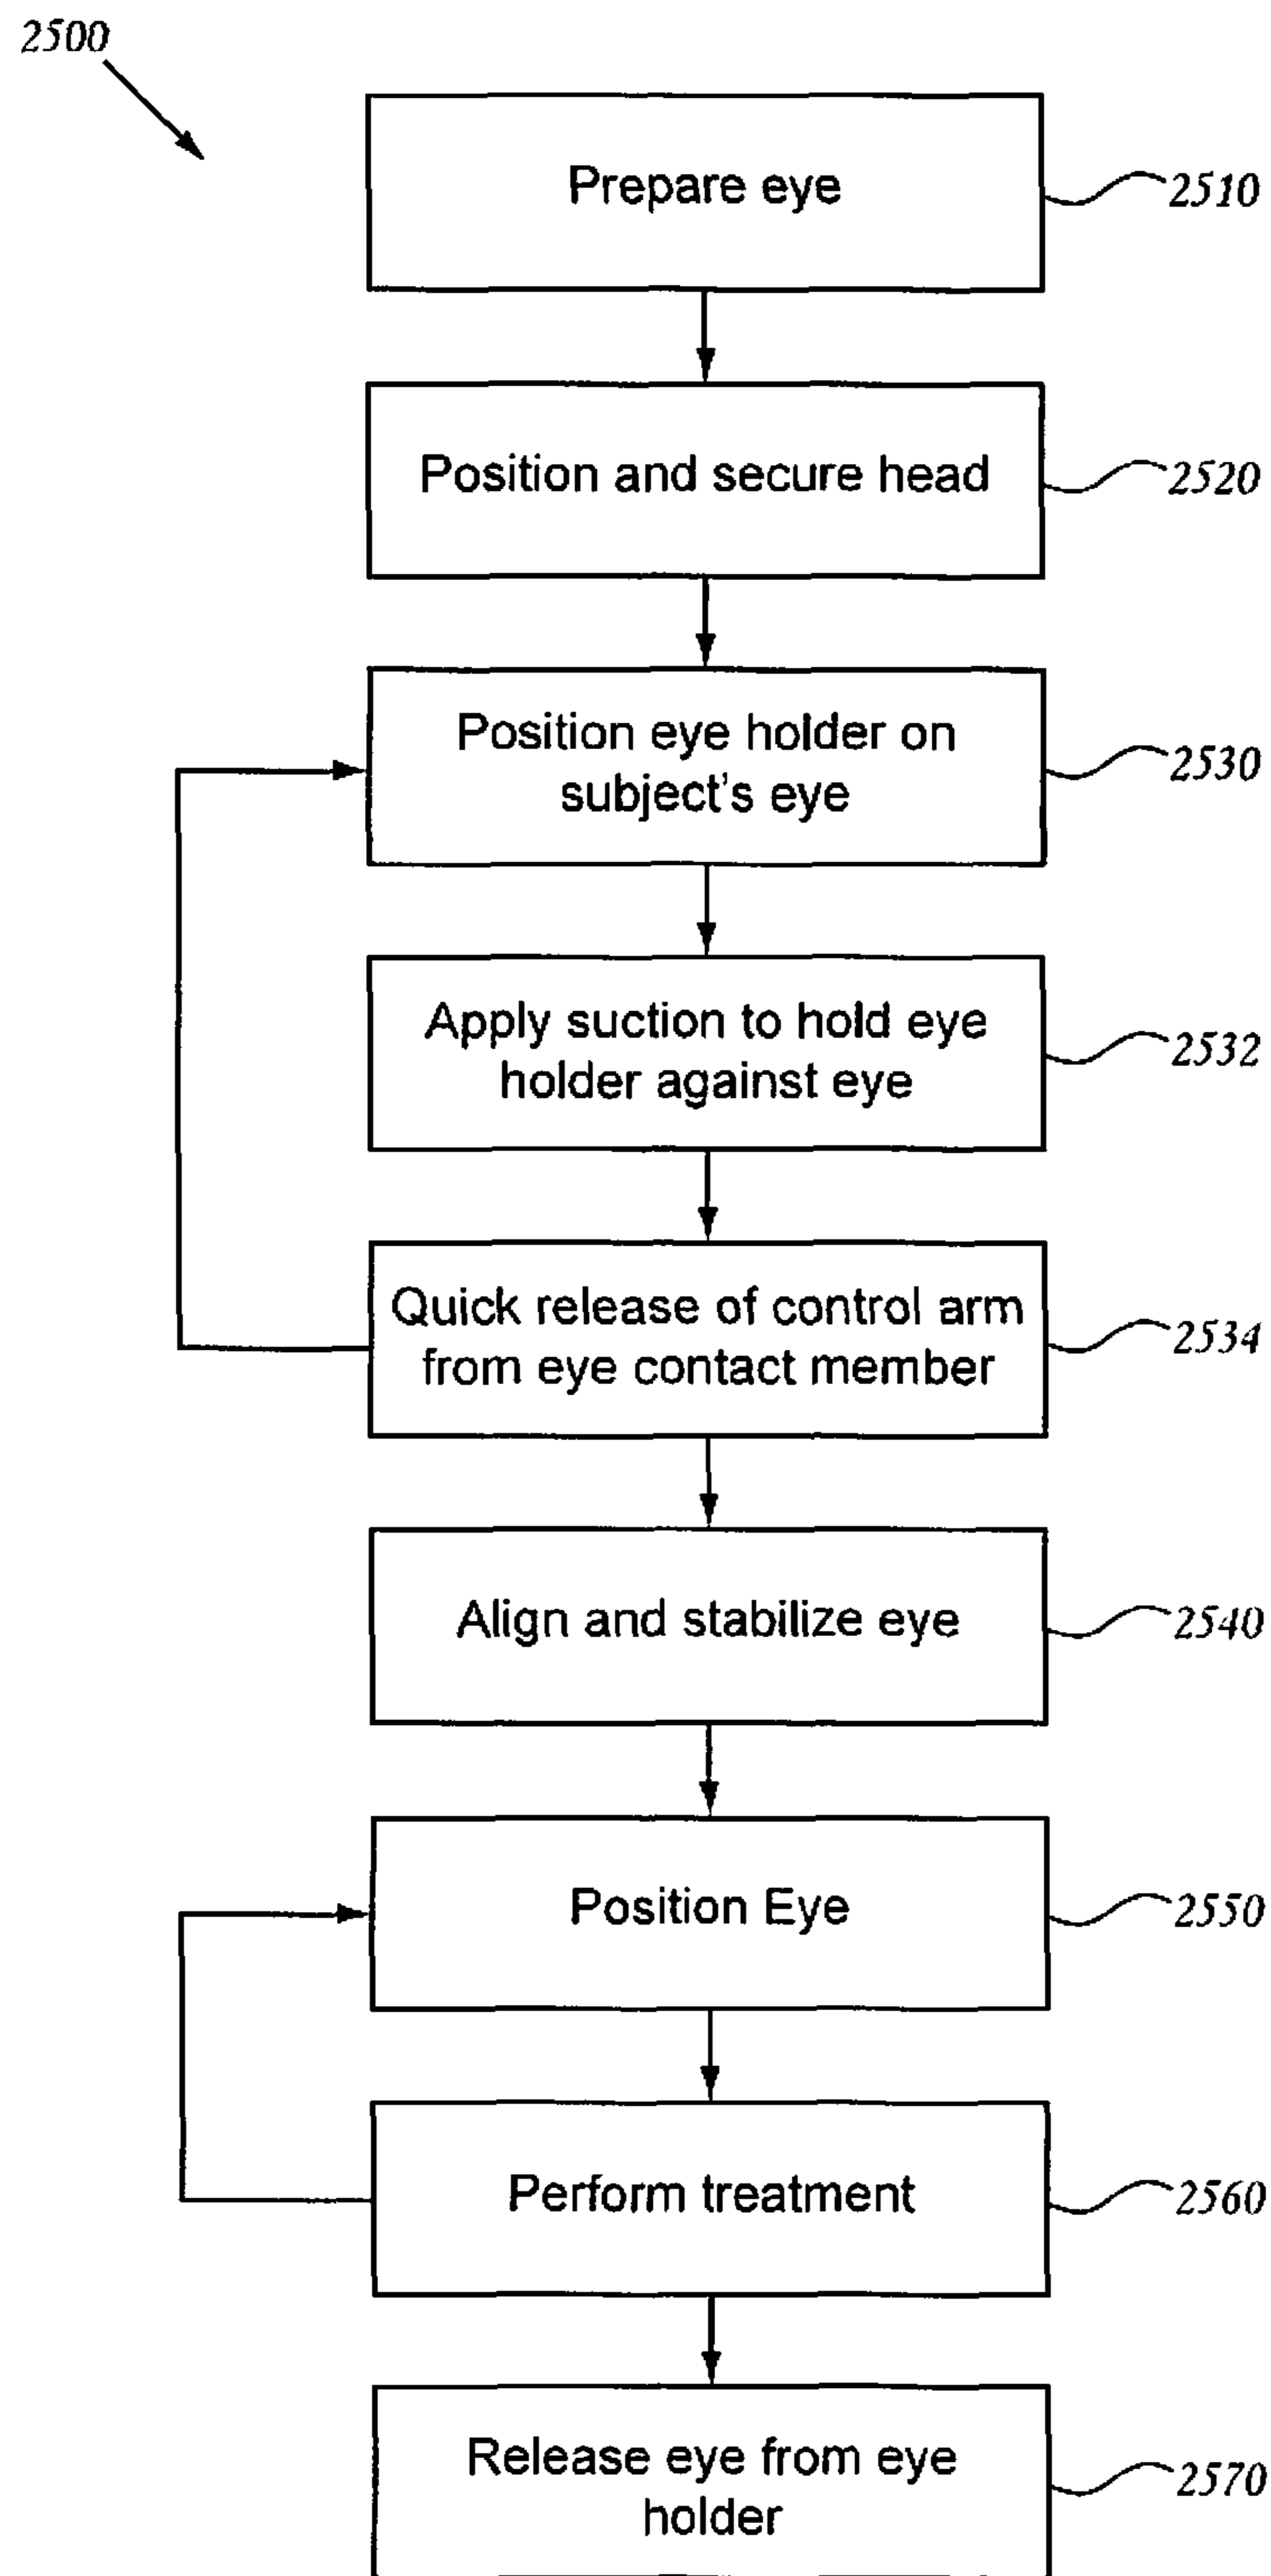


FIG. 25

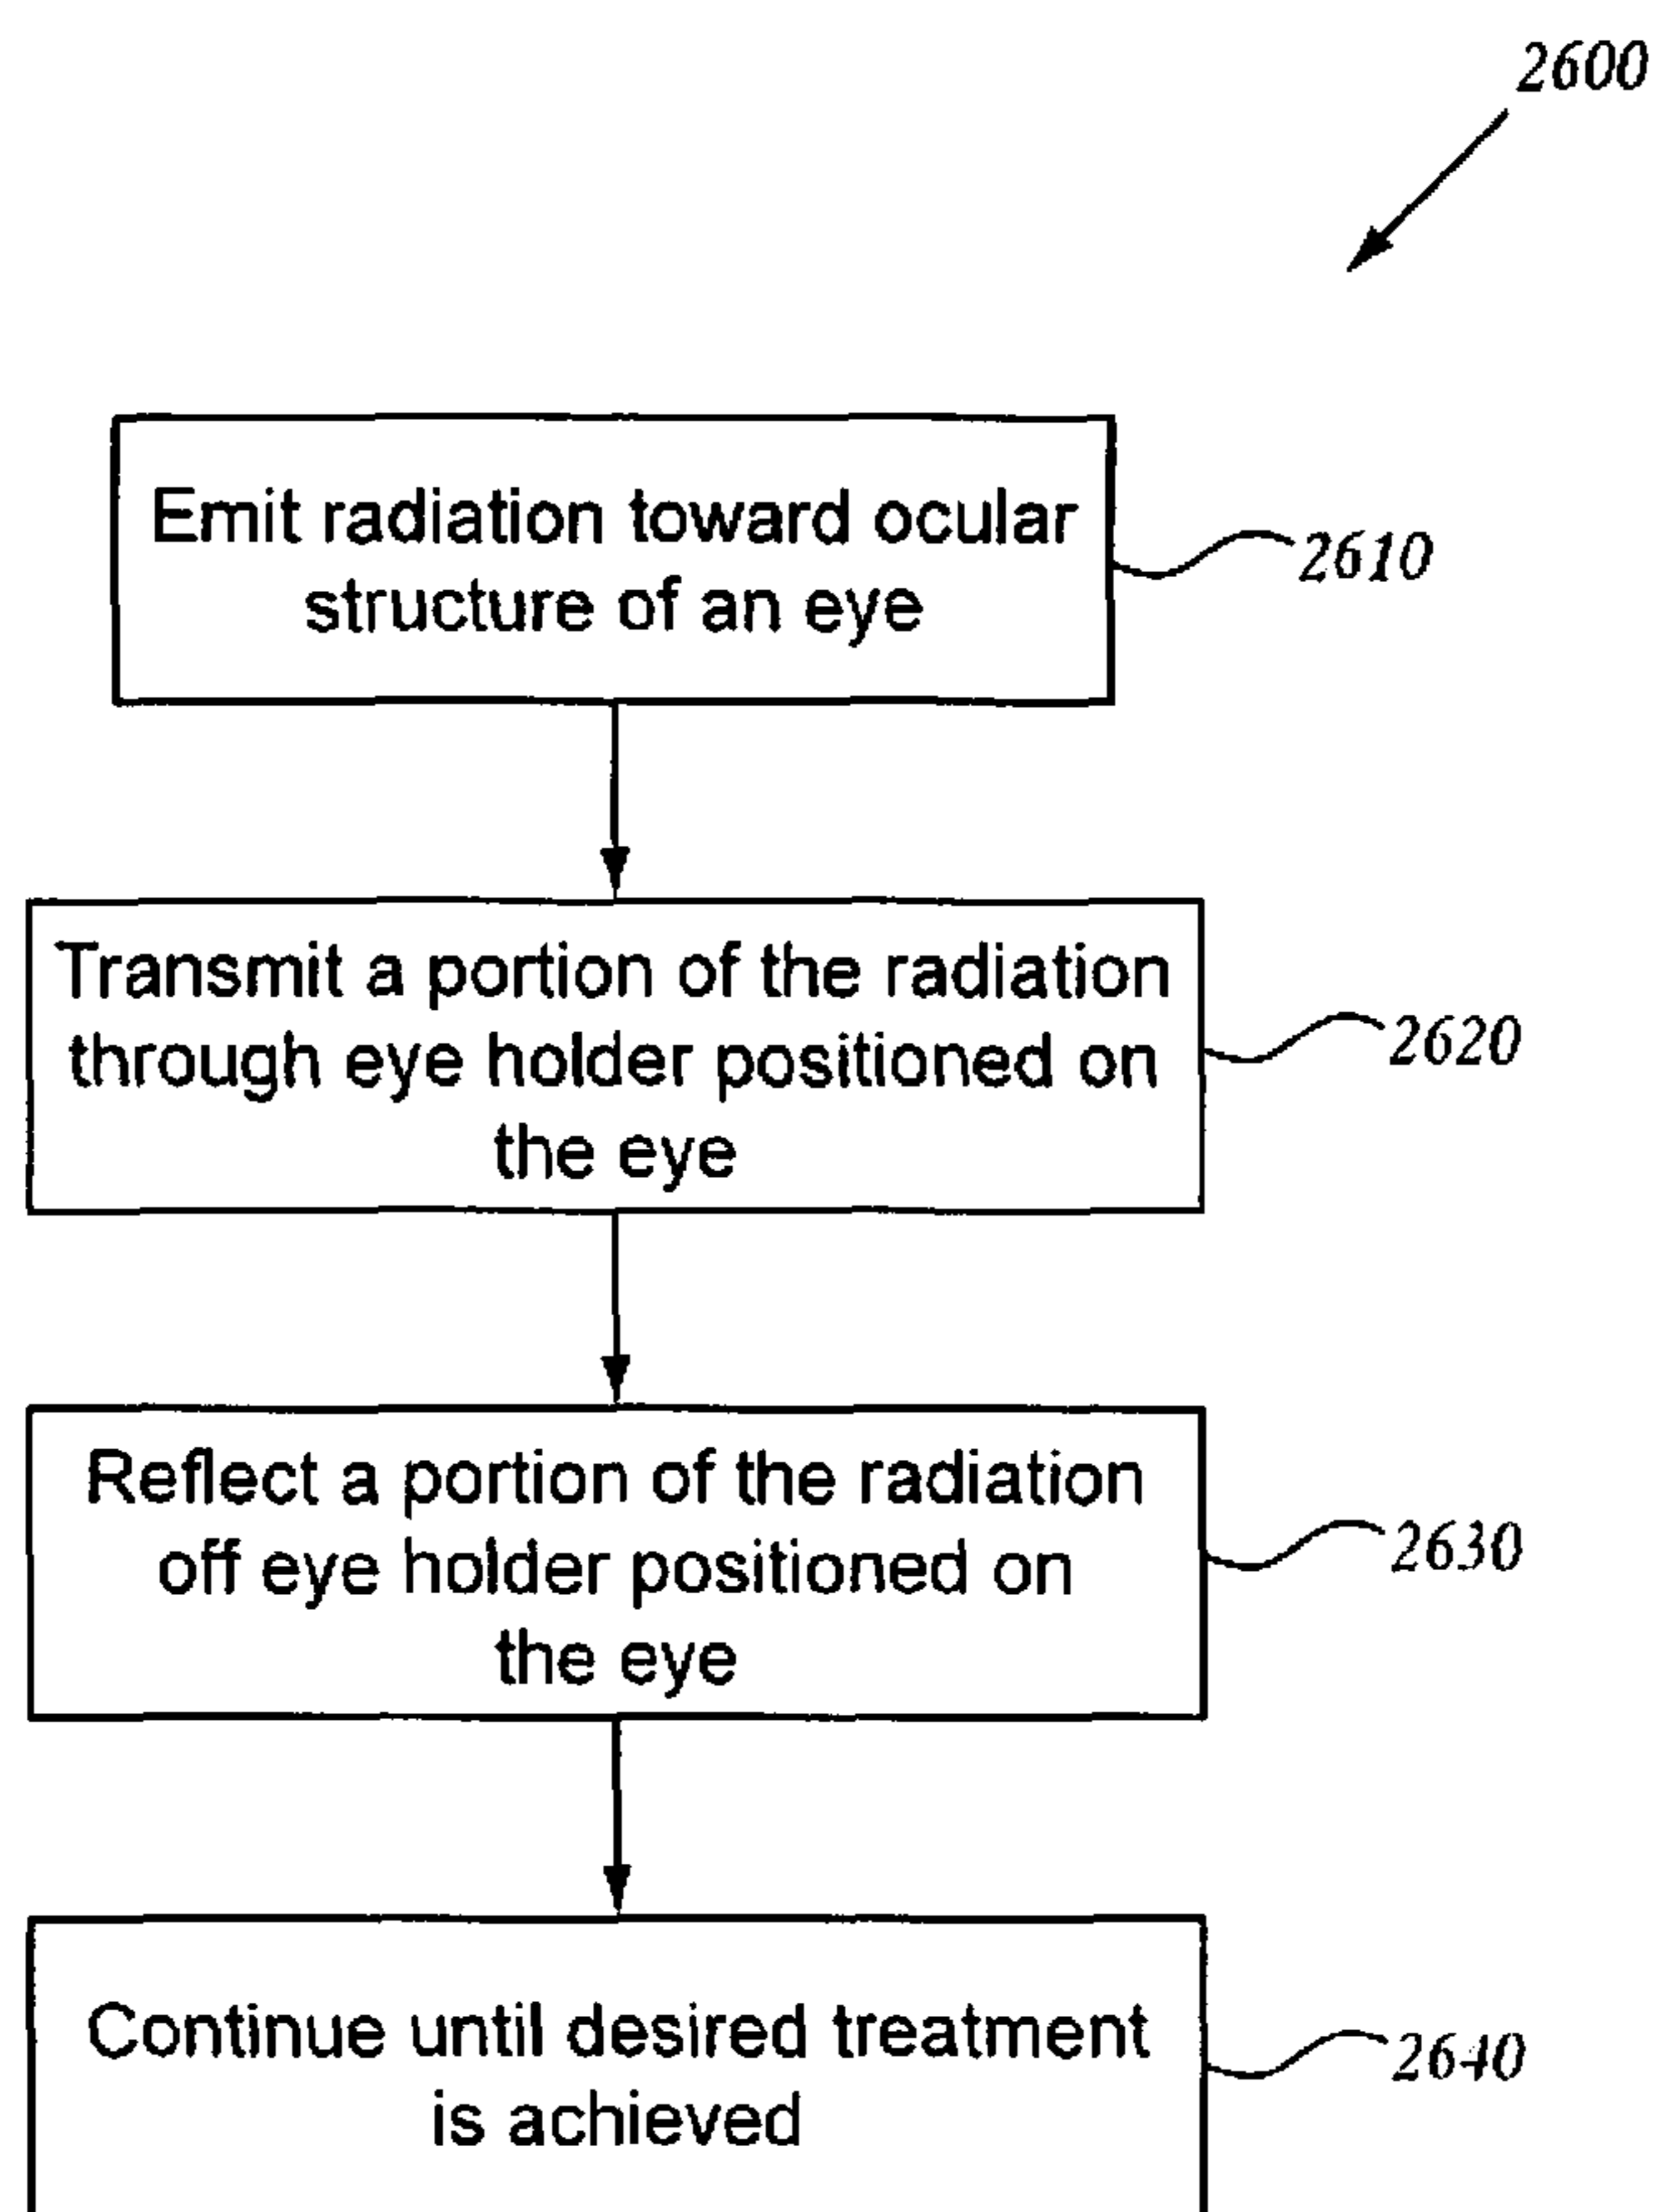


FIG. 26

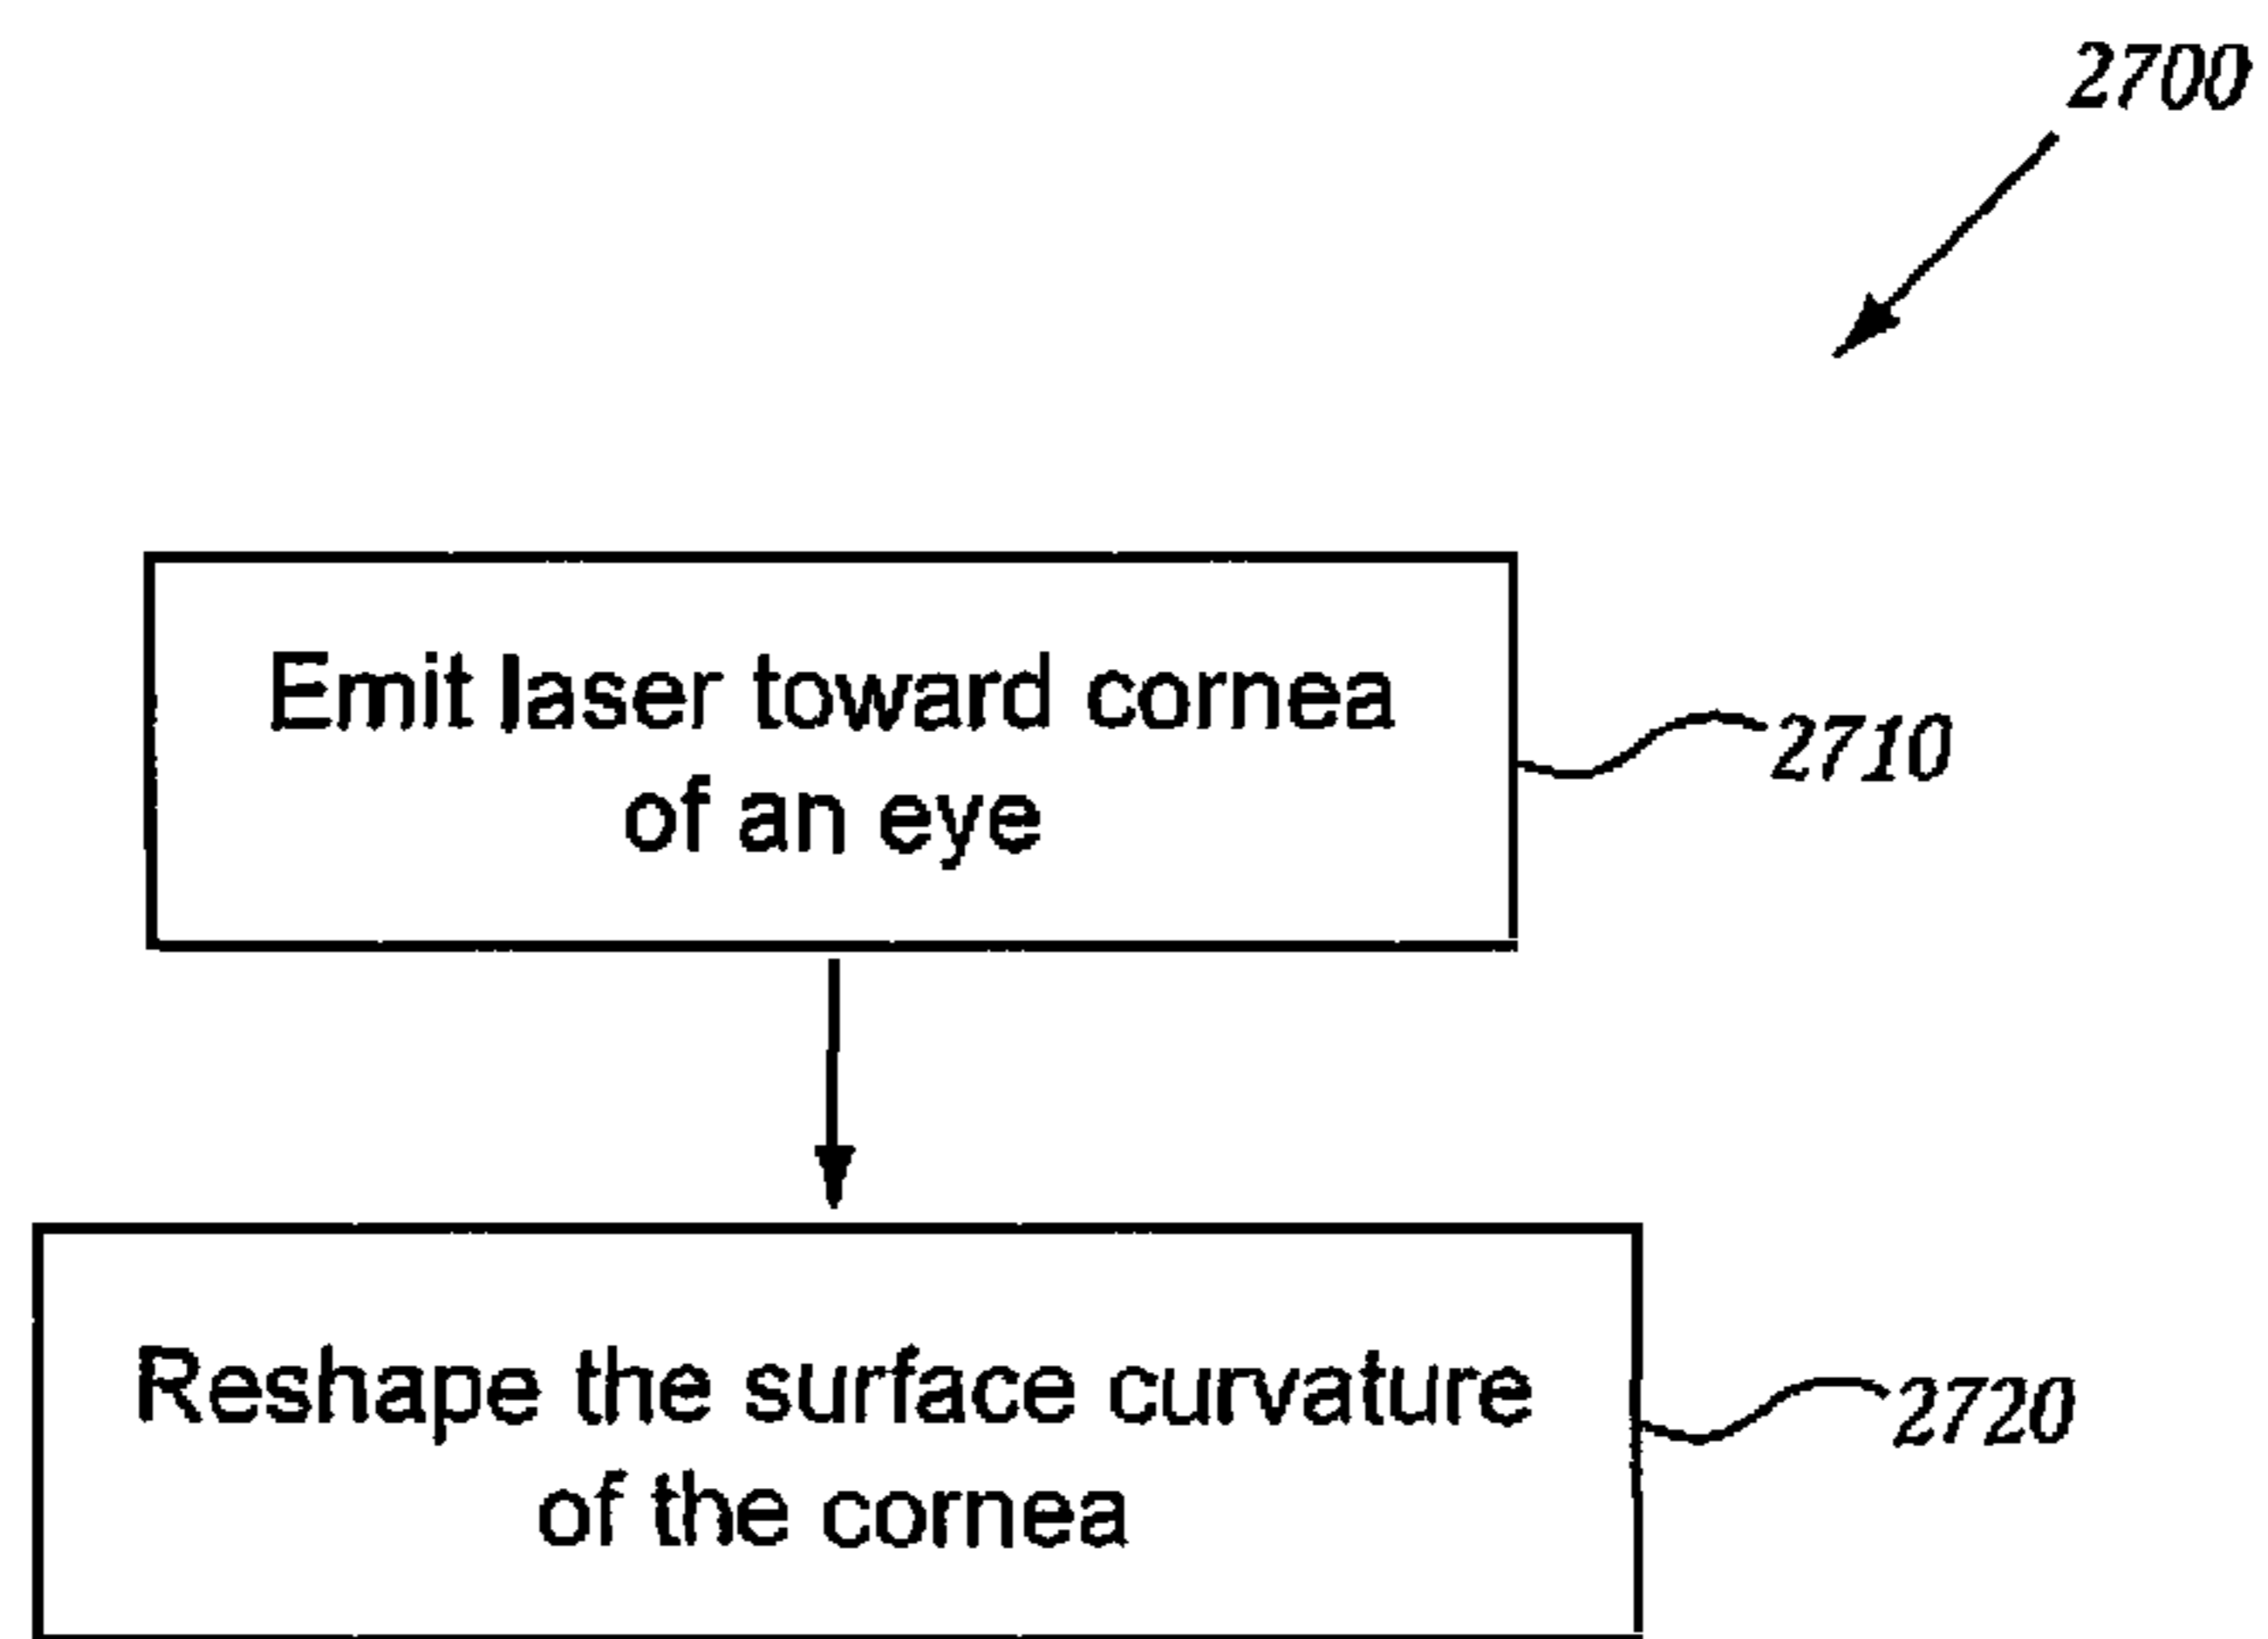


FIG. 27

## 1

**SYSTEM AND METHOD FOR PERFORMING  
AN OCULAR IRRADIATION PROCEDURE**

This application claims the benefit of priority to U.S. Provisional Patent Application No. 61/020,655 filed on Jan. 11, 2008, which is incorporated herein in its entirety by reference.

## FIELD OF THE INVENTION

The present invention pertains generally to a system and method for performing an ocular irradiation procedure on a patient's eye.

## BACKGROUND

A number of treatment and surgery procedures, typically involving irradiating one or more selected targets in the eye, require a patient's eye to be stabilized or positioned prior to and/or during treatment. For example, refractive laser surgery involves ablating corneal tissue of the eye with an ultra-fast, ultra-short pulse duration laser beam, to correct refractive errors in a patient's eye. To achieve ablation, refractive laser surgery requires a laser beam to be precisely focused to a very small focal spot within the cornea. As such, the patient's eye must be stabilized, and either the laser system must be properly and precisely aligned with the patient's eye, or the patient's eye must be properly and precisely aligned with the laser system.

In order to achieve proper alignment of the eye of the patient relative to the laser system, the system alignment settings and operating parameters must be well defined, steadfastly maintained, and frequently verified. Accurate and precise refractive surgery requires the corneal tissue be photoablated when the eye is substantially stabilized or stationary. Patient comfort and safety are also a consideration when holding the eye stationary and conducting laser surgery. Likewise, ocular radiotherapy treatment requires the eye to be stabilized and dynamically positioned during treatment.

In order to achieve the goal of maximizing results while minimizing risks to the patient during such eye treatment, it is important to eliminate, or at least significantly reduce, as many system errors as possible. This includes the improper alignment of the patient's eye relative to the treatment system. Alignment errors may result from either a misconfiguration of the system, or from the patient's interaction with the system. Insofar as patient/system interaction is concerned, any voluntary or involuntary movement of the patient's eye during treatment can significantly alter the alignment of the eye relative to the treatment system. It is necessary, therefore, to hold the eye of the patient stationary during these procedures.

In addition to the operational issues discussed above, patient safety is also a concern. In particular, when the eye is in direct contact with the system, the magnitude of the interactive forces that are exerted on the eye are of concern. The variety of events that can cause these forces to exceed safety limits need to be avoided. Thus, there is a need for a system which can physically manipulate the position of the eye, prevent undesired eye movement during treatment, provide needed safety precautions, and function as a positional reference between the surface of the eye, selected internal anatomy of the eye (e.g., the macula or optic nerve), and the system. The present system is designed to meet these needs.

## SUMMARY OF THE INVENTION

The invention includes, in one embodiment, a system for performing an ocular irradiation procedure on a patient's eye.

## 2

The system includes (a) a head support for supporting the patient's head, (b) an eye-contact device attachable to the front portion of the patient's eye, to stabilize the position of the eye relative to the eye-contact device; (c) means for determining the position of the patient's eye, with such stabilized with respect to the contact device, and with the patient's head supported in the head support, in an external coordinate system, (d) a source of a collimated irradiation beam, and (e) a beam-positioning assembly for positioning the beam source in the external coordinate system such that the beam, when activated, is aimed along a selected path at a selected coordinate in the external coordinate system corresponding to a selected target region in the patient's eye.

The eye-contact device may include an internal concave eye-contact surface adapted to be placed against the front surface of a patient's eye, an external surface, a port in fluid communication with the contact surface, by which a negative pressure, e.g., a vacuum of between about 20 to 50 Hg, can be applied between the eye and the contact surface, to stabilize the position of the eye with respect to the contact device, and a connector carried on the outer surface of the device. In this embodiment, the system may further include a biasing mechanism operatively connected to the connector of the contact device for biasing the contact device against the eye with a force sufficient to hold the contact device against the eye, when the eye is stabilized with respect to the device by application of a negative pressure between the eye and the device's contact surface. An exemplary force is between 1-25, typically 5-20, gram-force.

The determining means may include a position detector for determining the position of the contact device, and thus the position of the patient's eye attached to the contact device, in the external coordinate system. In this general embodiment, the position detector may include a plurality of beam elements mounted on the contact device, for directing beams in accordance with the position and orientation of the beam elements, sensors for detecting the directions of the beams, and a processor for determining from the detected beam directions, the position and orientation of the contact device in the external coordinate system.

The system may further include an eye-positioning assembly for moving the eye-contact device to place the device at a selected position in the external coordinate system, and the position detector may be operable to determine the position of the contact device in the external coordinate system, with such placed at said selected position. The eye-positioning assembly may be operable to adjust the angular position of the contact member with respect to the patient's head, and the position detector may detect an angle of a beam emanating from the contact member. The eye-positioning assembly may include an arm that is pivotally attached to the eye-contact member, and an arm control mechanism for controlling the movement of the arm in at least one direction in the external coordinate system, and the position detector may be operable to determine the position of the contact device in the external coordinate system from the position of the eye-positioning assembly arm in the external coordinate system.

The determining means includes a reference-beam light source operatively connected to the irradiation-beam source, for producing a reference light beam along a path coincident with the collimated irradiation beam produced by the irradiation beam source, and the beam-positioning assembly may be operable to place the irradiation beam source at a position such that the collimated light beam is aimed at the selected target region of patient's eye.

For use in treating macular degeneration in a patient eye, the beam source may be a source of soft collimated x-rays,

and the beam-position assembly may be operable to position the beam source to direct a collimated x-ray beam at the macular region of the eye, along a path through an outer side region of the eye that makes an angle with an axis normal to the cornea of the eye, between about 5 and 45 degrees.

In another embodiment, the invention includes a method for performing an ocular irradiation procedure on a patient's eye, by the steps of: (a) supporting the patient's head in a head support, (b) attaching to the front of the patient's eye, an eye-contact device effective to stabilize the position of the eye relative to the contact device; (c) with the eye-contact device placed to a selected position, and with the patient's head supported in the head support, determining the position of a selected target region of the patient's eye in an external coordinate system, (d) positioning a source of a collimated irradiating beam in the external coordinate system such that the source beam, when activated, is aimed along a selected path at a selected coordinate in the external coordinate system corresponding to a selected target region in the patient's eye, and (e) activating the beam source.

Attaching step (b) may include placing against the front portion of the patient's eye, a concave contacting surface of an eye-contact device, and applying a negative pressure between the eye and the contact surface, thus to stabilize the position of the eye with respect to the contact device, and which further includes biasing the contact device against the eye with a force sufficient to hold the contact device against the eye, wherein the position of the eye is stabilized with respect to the device. The negative pressure applied to the contact device may be between 20 mm Hg and about 50 mm Hg. An exemplary force is between 1-25, typically 5-20, gram-force.

The method may further include, after attaching the eye to the eye-contact device, moving the contact device to place the device at a selected position in the external coordinate system, and step (c) may include determining the position of the ocular device in the external coordinate system, with such placed at its selected position. Moving the eye-contact device to place the device at a selected position in the external coordinate system may include directing an incident light beam onto a reflective surface of the contact member, detecting the angle of the beam reflected from said surface, and adjusting the angular position of the contact member until the incident light beam is coincident with the reflected light beam.

Determining the position of a selected target region of the patient's eye in an external coordinate system includes aiming a collimated light beam along a path coincident with the collimated electromagnetic beam produced by the beam source and positioning the light beam until it is aimed at the selected target region of patient's eye.

For use in treating macular degeneration in a patient eye, step (d) may include positioning a collimated x-ray beam source to direct a collimated x-ray beam at the macular region of the eye, along a selected path through an outer side region of the eye that makes an angle with an axis normal to and through the center of the cornea of the eye, of between about 5 and 45 degrees. The treatment method may include repeating steps (d) and (e) at each of a plurality of different paths of the collimated x-ray beam.

These and other objects and features of the invention will be more fully appreciated when the following detailed description of the invention is read in conjunction with the accompanying figures.

#### BRIEF DESCRIPTION OF THE FIGURES

The figures and the associated descriptions are provided to illustrate embodiments of the disclosure and not to limit the

scope of the disclosure. Throughout the figures, reference numbers are reused to indicate correspondence between referenced elements. The figures are in simplified form and are not necessarily precise in scale. In reference to the disclosure herein, for purposes of convenience and clarity only, directional terms, such as top, bottom, left, right, up, down, over, above, below, beneath, rear, and front are used with respect to the accompanying figures. Such directional terms are not to be construed as limiting the scope of the invention in any manner.

FIG. 1 illustrates a top view of one embodiment of a system for controllably positioning and/or stabilizing the eye of a subject for therapeutic treatment;

FIGS. 2A-2B illustrate top views of an embodiment of a system for engaging the eye of a subject;

FIGS. 3A-3D illustrate top and perspective views of the contact device and pivotable control arm in accordance with preferred embodiments of the invention;

FIGS. 4A-4F depict an exploded view (FIG. 4A), connecting views (FIGS. 4B-4E), and another view (FIG. 4F) of the contact device in accordance with certain embodiments of the invention;

FIGS. 5A-5B depict perspective views of the contact device without the control arm attached (FIG. 5A) and with the control arm attached (FIG. 5B) in accordance with preferred embodiments of the invention;

FIGS. 6A-6C depict perspective views of an contact device and control arm being reversibly engaged with the system in accordance with one embodiment of the invention;

FIGS. 7A-7C illustrate a method of engaging and positioning an eye of a subject in accordance with one embodiment of the invention;

FIGS. 8A-8B illustrate perspective views of the contact device out of alignment with the system (FIG. 8A) and in substantial alignment with the system (FIG. 8B) in accordance with preferred embodiments of the invention;

FIG. 9 is a frontal plan view of an embodiment of an eye-contact member with no aperture included within the eye-contact member;

FIG. 10 is a frontal plan view of an embodiment of an eye-contact member with a circular shaped aperture offset from the center of the eye-contact member;

FIG. 11 is a frontal plan view of an embodiment of an eye-contact member with an irregular shaped aperture offset from the center of the eye-contact member;

FIG. 12 is a frontal plan view of an embodiment of an eye-contact member with a heptagonal shaped aperture offset from the center of the eye-contact member;

FIG. 13 is a frontal plan view of an embodiment of an eye-contact member with a plurality of circular shaped apertures offset from the center of the eye-contact member;

FIG. 14 is a frontal plan view of an embodiment of an eye-contact member with a diamond shaped aperture offset from the center of the eye-contact member;

FIG. 15 is a frontal plan view of an embodiment of an eye-contact member with a circular shaped aperture offset from the center, and located at the edge, of the eye-contact member;

FIG. 16 is a frontal plan view of an embodiment of an eye-contact member with a kidney shaped aperture offset from the center of the eye-contact member;

FIG. 17 is a frontal plan view of an embodiment of an eye-contact member with a circular shaped aperture offset from the center, and located at the edge, of the eye-contact member;

FIGS. 18A-B are frontal plan views of embodiments of an eye-contact member with up to one half of the eye-contact

5

member removed (FIG. 18A), and more than one half of the eye-contact member removed (FIG. 18B);

FIG. 19 is a frontal plan view of an embodiment of an eye-contact member with a plurality of radially extending slots emanating from the center of the eye-contact member;

FIG. 20 is a side view of the eye-contact member of FIG. 19 showing a plurality of radially extending slots emanating from the center of the eye-contact member;

FIG. 21 is a frontal plan view of an embodiment of an eye-contact member with a plurality of circular shaped apertures increasing in size and radially spaced from the center of the eye-contact member;

FIG. 22 is a side view of the eye-contact member of FIG. 21 showing a plurality of circular shaped apertures increasing in size and radially spaced from the center of the eye-contact member;

FIG. 23 is a frontal plan view of an embodiment of an eye-contact member with a grid of apertures within the eye-contact member;

FIG. 24 is a side view of the eye-contact member of FIG. 23 showing a grid of apertures within the eye-contact member;

FIG. 25 is a flow chart illustrating one method of utilizing the system for stabilizing and positioning an eye for treatment;

FIG. 26 is a flow chart illustrating a method of utilizing the system for treating an eye with radiation in accordance with one embodiment of the invention; and

FIG. 27 is a flow chart illustrating a method of utilizing the system for laser treating an eye in accordance with another embodiment of the invention.

## DETAILED DESCRIPTION

Reference will now be made in detail to disclosed embodiments of the invention, examples of which are illustrated in the accompanying figures.

### I. Definitions

Unless otherwise indicated, all technical and scientific terms used herein have the same meaning as they would to one skilled in the art of the present invention. It is to be understood that this invention is not limited to the particular methodology and protocols described, as these may vary.

As used herein, “accommodation” refers to the ability to change focus from distant objects to near objects, which ability may tend to diminish with age.

The term “choroid” refers to the highly vascular layer of the eye beneath the sclera.

As used herein, “ciliary muscle” refers to a muscular ring of tissue located beneath the sclera and attached to the lens via zonules.

As used herein, “conjunctiva” refers to the thin, transparent tissue covering the outside of the sclera. In some embodiments of the invention, reference is made to one or more devices or systems of the invention in contact with outer structures of the eye, such as the sclera. In these embodiments, it is to be understood that the device or systems of the invention may be in contact with the named structure, or may be in contact with the conjunctiva covering the structure.

As used herein, “cornea” refers to the transparent, avascular tissue that is continuous with the opaque sclera and semi-transparent conjunctiva, and covered by tear film, or corneal epithelium, on its anterior surface and bathed by aqueous humor on its posterior surface.

As used herein, “limbus” refers to the boundary where the cornea meets the sclera.

6

As used herein, “retina” refers to the light-sensitive layer of tissue that lines the inner back of the eye and sends visual impulses through the optic nerve to the brain.

As used herein “ocular disease” refers to a disease of the eye, including, but not limited to tumors, ocular degeneration, such as macular degeneration retinopathies, retinitis, retinal vasculopathies, diabetic retinopathies, diseases of the Bruch’s membrane and the like.

As used herein, the term “reducing ocular disease” also encompasses treating and alleviating the ocular disease.

As used herein, “sclera” refers to the outer supporting structure, or “white,” of the eye.

As used herein, the “front of the eye” refers at least a central portion of the cornea and may include surrounding structures, such as the sclera.

As used herein, the term “subject” refers to man or any animal that has eyes.

As used herein, “vitreous body” refers to the clear colorless transparent jelly that fills the eye posterior to the lens and that is enclosed by a hyaloid membrane.

As used herein, “zonules” refers to a circular assembly of radially directed collagenous fibers that are attached at their ends to the lens and at their outer ends to the ciliary muscle.

As used herein, the term “presbyopia,” refers to the inability of the eye to focus sharply on nearby objects. Presbyopia is associated with advancing age and typically entails a decrease in accommodation. Introduction of treatment, e.g., laser ablation, according to any of the implementations described herein, preferably increases or facilitates an increase in accommodation, thereby mitigating effects of presbyopia.

The term “radiodynamic therapy” refers to the combination of collimated x-rays with a concomitantly administered systemic therapy.

The term “radiodynamic agents” is intended to have its ordinary and plain meaning, which includes, without limitation, agents that respond to radiation, such as x-rays, and agents that sensitize a tissue to the effects of radiation.

The term “photodynamic therapy” refers to a therapeutic or diagnostic method involving use of a photoreactive agent and radiation of a sufficient intensity and wavelength to activate the photoreactive agent. The activated photoreactive agent then, through emission of energy, exerts a therapeutic effect or allows for diagnosis through detection of emitted energy.

The term “photodynamic agents” is intended to have its plain and ordinary meaning, which includes, without limitation, agents that react to light and agents that sensitize a tissue to the effects of light.

The term “radiation therapy” is intended to have its well-accepted meaning and can also refer to any treatment performed with an energy source.

As used herein, “treatment” refers to any manner in which one or more of the symptoms of a disease or disorder are ameliorated or otherwise beneficially altered. Treatment also encompasses any therapeutic use of the systems herein.

As used herein the term “external coordinate system” refers to a coordinate system that is fixed, such as a room or the fixed element, e.g., base, of a system component. It typically provides a common set of coordinates to place in registry, devices which are moving relative to one another, or which cannot be accurately placed at pre-selected position in the coordinate system, such as a patient’s head.

Diagnostics can also be performed with any type of energy source or treatment described herein and may be referred to as “radiation diagnostics.”

The “position” of an object, such as an eye-contact member, in an external coordinate system refers to the position of

some known point on the object, as defined by the coordinates of that point in the coordinate system. The coordinate system may be, for example, a three-dimensional Cartesian coordinate system, in which the object's position is defined by x, y, and z coordinates, or a spherical coordinate system in which object's position is defined by radius and angle coordinates.

A "biasing force" refers to a force exerted against a patient's head (or eye), typically expressed in terms of units of gram-force, i.e., the force exerted by the earth's gravity acting on a gram mass.

A "beam-directing element" refers to an element capable of reflecting an impinging beam, such as a light, microwave, or ultrasound beam, onto a detector, or an element that itself is capable of producing a beam, such as a light beam that is aimed at one or more beam detectors. The beam-directed elements are attached to an eye-contact device or assembly for purposes of determining the positions of the beam-directing elements, and thus the position of an eye-contact device or assembly to which they are attached, in an external coordinate system.

A "reservoir" or "vacuum reservoir" refers to an internal chamber or chambers, e.g., array of fluid-carrying tubes, by which a negative pressure applied to an eye-contact device can be distributed over the contact surface of an eye-contact member.

A "pivot joint" refers to a coupling between two mechanical elements that allow of the elements to shift, typically in an angular direction, with respect to the other element. Exemplary pivot joints include ball and universal joints, both of which provide multiple degrees of freedom, e.g., degrees of angular motion, between the two elements.

## II. System for Stabilizing the Eye and for Performing an Ocular Irradiation Procedure

A system in accordance with the present invention is shown in FIG. 1 and is generally designated **100**. The system **100** functions as an ocular interface useful for one or more of the following functions: i. controllably stabilizing the eye; ii. physically manipulating eye position; iii. limiting eye from movement during treatment; iv. positionally referencing the surface of the eye, its internal anatomy, and/or the system (e.g. to an external coordinate system) v. providing fiducials relative to the eye and relative to treatments performed as well as monitoring positioning of the fiducials relative to the eye; vi. maintaining corneal lubrication during treatment; vii. provide a mechanism to align a treatment device and continuously signal adequate alignment or misalignment. Substantial or total controllable stabilization of the eye is advantageous for a wide variety of treatment, diagnostic, and/or surgery procedures as described in detail below.

The system **100** includes a platform **105** which allows stationary attachment of one or more of the components of the system, as described below, such that precise positional information regarding the components of the system relative to a known coordinate system (e.g., an external coordinate system) are capable of being determined. The system defines a reference or external coordinate system in which the components of the system are registered, such that all of the points can be positioned and aligned with one another at known positions in the external coordinate system. The components of the system described may be automatically positioned in the coordinate system by a computer interface, as will be described below. Alternatively, some of the components of the system **100** may be manually positioned. In another embodiment, one or more of the components of the system

**100** are positioned automatically, and one or more of the components of the system **100** are simultaneously positioned manually.

System **100** includes an eye-contact device **110** having an eye-contact member or surface **120** that reversibly engages or couples to the front of an eye **130** of a subject **140** (e.g., FIGS. 2A and 2B). Contact device **110** is connected to a control arm **180** which is part of an eye-positioning assembly **182** for placing the contact device at a selected position in the external coordinate system, as will be seen below. Preferably, control arm **180** is pivotably connected to contact device **110** as described below. In some embodiments, the control arm releasably detach from the contact device or the eye-contact member in case of sudden patient movement, as will be described below with respect to FIGS. 4A-4D. The eye-contact member **120** engagement with the eye **130** maintains the eye in substantially stabilized or immobilized position. Alignment of the eye can be accomplished with the use of the laser device **150**, which can provide alignment of the contact device **110** as described in further detail below. Thus, FIG. 1 illustrates a preferred embodiment of the patient ocular interface system **100** of the invention.

With continuing reference to FIG. 1, system **100** is a patient ocular interface for treatment of an ocular structure with a treatment device **160**. As noted, the system includes an eye-contact device **110** adapted to maintain an eye **130** in a substantially stable position. In one embodiment of the invention, the contact device is configured to provide an indication to a sensor that the eye **130** is in substantially the first position during delivery of treatment from device **160**, located outside the eye. In a preferred embodiment, the system includes a communication link **185** that communicates information between the contact device **110** and the treatment device **160**, the information being indicative of a position of the eye and determining a characteristic of one or more parameters of the treatment device **160**.

Treatment device **160** may include any of a number of devices that provide therapeutic treatment to the eye. Such therapeutic treatments are described in detail below. In general, device **160** is a source or a collimated irradiation beam directed along a selected axis or path **168**, such as a source of electromagnetic radiation (e.g., ablating optical energy, thermal optical energy, low level therapeutic optical energy, or radiofrequency energy), ultrasound, and magnetic implementations. The treatment device **160** includes, in one general embodiment, is an energy emitting source, such as an electromagnetic laser (e.g., a diode laser) and/or radiation source having a predetermined wavelength, an ultrasound device with a predetermined pulse, a cautery device with a predetermined setting that interacts with desired parts of the eye, a radiofrequency module, an ultrasonic component, and combinations thereof. Device **160** can further be a surgical implement or manipulator; for example, a surgical probe for intraocular brachytherapy or superficial brachytherapy can be held in position in a similar manner as device **160** with the exception that the surgical implement is placed inside the eye. In one preferred embodiment of the invention, the treatment device **160** is a source of a collimated irradiation beam, such as a portable source of soft-x-ray beams generated by directing soft x-rays from a conventional x-ray source through a collimator. For purposes of illustration, device **160** will be referred to herebelow as a source **160** of a collimated irradiation beam.

Device **160**, in some embodiments, can be a diagnostic device. It may be desirable to hold an eye in a position to obtain fine detailed diagnostic information about the eye such as OCT, scanning laser ophthalmoscopy, CT scan, MRI, or



any other device which may send energy into the eye and be dependent on steadiness of the structure and/or a known coordinate reference.

A beam-positioning assembly **162** in the system is designed to position the beam source **160** in the external coordinate system such that the beam, when activated, is aimed along a selected path, corresponding to the beam axis **168**, at a selected position in the external coordinate system corresponding to a selected target region of the patient's eye. As seen in FIG. **1**, the beam-positioning assembly includes a swivel mount **164** on which the beam source is mounted for rotation about an axis **163**, and a linear guide **166** on which the swivel mount can travel along an axis **167**. Although not shown here, the "height" position of the beam source can be adjusted along axis **163**, so that the beam from the beam source is at the same height as a target region in the patient eye. The angular position of the beam source position on swivel mount **164** and the linear position of the swivel mount on guide **166** can be adjusted manually, or preferably, is under the control of stepper or servo motors which themselves are controlled by a control unit **115**, described below. In addition, the mounting on the beam source on swivel mount **164** may be through a connection, such as a ball or universal joint, that allows the angle of the beam-source collimated beam, represented by axis **168**, to be adjusted "up" or "down" with respect to a the plane representing by platform **105**, for directing the beam at slight upward or downward angles into the eye.

A head support or support **170** for stabilizing the head of subject **140** is included in system **100**, and includes a chin rest **172** (FIGS. **8A** and **8B**). Head support **170** is, in the embodiment of the invention illustrated in FIG. **1**, attached to the platform **105**, e.g., by permanent or releasable attachment. In one embodiment, head support **170** includes a motorized control assembly with position sensors which can be selectively activated to move and reconfigure the head support. Further details of the support, and its function is supporting a patient's head, is described below with respect to FIGS. **8A** and **8B**.

Also included in the system are means for determining the position of a selected target region of the patient's eye in the external coordinate system, with the patient's eye stabilized with respect to the eye-contact device, and the contact device moved to a selected position. The coordinate or coordinates thus determined are used by the beam-positioning assembly to move the beam source in the external coordinate system such that the collimated irradiation beam, when activated, is aimed along a selected path at the selected eye coordinate corresponding to the selected target region of the patient's eye in the external coordinate system.

In a first general embodiment, the means for determining the position of a selected eye target includes an eye-positioning assembly illustrated in FIGS. **6A-6C**, for positioning the eye-contact device at a selected orientation or alignment, a detector for determining when the eye-contact device has been moved to the selected orientation, and position sensors in the eye-positioning assembly for determining the coordinates of the eye-contact device when moved to the selected orientation. In particular, FIGS. **8A** and **8B** depict a mechanism by which the contact device **110** can be used to align the eye with laser alignment system **800**, including laser device **150**. Optionally, the alignment mechanism also directly aligns a treatment system, such as a radiotherapy system (not shown) in which the radiotherapy system directs its energy toward the eye in relation to the alignment system. Laser pointer beam **810** (which is collinear with the therapeutic beam in some embodiments) is emitted from laser system **800**

through a collimator opening **820** and reflects off the surface of beam-directing mirror **230** of the contact device **110**. In the non-alignment case depicted in FIG. **8A**, the laser pointer beam **810** will not reflect off the surface of mirror **230** collinearly with the collimator opening **820**, but will be off-axis, as shown by reflection beam **830**. The orientation of the laser system **800** and/or the contact device **600** can be manually or automatically adjusted by direct visualization of the location of the reflection beam **830** or by sensors that detect the location of the reflection beam **830** and adjust the laser system **800** to bring the laser reflection beam **830** into alignment. In the case where the laser pointer is in fact aligned (FIG. **8B**), the laser pointer beam **810** is reflected, and the laser reflection beam **830** is substantially collinear with the laser pointer beam **830**.

The eye-positioning assembly used to position the eye-contact device at a selected orientation, as just described, is illustrated in FIGS. **6A-6C**. The figures show perspective views of the contact device **110** attached to a control arm **180** in the positioning assembly, indicated at **625**, which is being fed into slot **610** of drive mechanism **600**. In some embodiments, the contact device **110** of the system can be attached to a coupling component to hold the eye in place. The coupling component can be attached to the treatment device, but preferably, as shown in FIGS. **6A-6C**, it is attached at a location separate from the radiotherapy device, such as a drive mechanism **600** that is attached to a table or platform **620** which holds the treatment device.

Contact device **110** is preferably disposable such that a separate (e.g. disposable) contact device **110** is employed for each subject and/or use. Alternatively, contact device **110** may be nondisposable and be treated, e.g., with anti-infective agents, prior to being utilized in multiple subjects' eyes. Drive mechanism **600** is fixed to base **620** through connector **640**, which is may robotically controlled, but preferably manually controlled, and has a known coordinate system. In one embodiment, drive mechanism **600** is fixed in a known, or predetermined, location with respect to the head positioning system (not shown) and/or the eye of the subject (not shown) and/or the positioning system of the radiotherapy device. Push button **630** allows free manual positioning of contact device **110** into and/or out of slot **610**. Thus, as illustrated in FIG. **6A**, the control arm **180** is not engaged with the drive mechanism **600**. In FIG. **6B**, the control arm **180** is partially engaged with the drive mechanism **600**. And in FIG. **6C**, the control arm **180** is fully engaged with the drive mechanism **600** and is fixed in a known, or predetermined location, which allows the eye of the subject to be fixed in a known, or predetermined location, when contact device **110** engages the eye.

Although not shown, the eye-positioning device includes internal position sensors operable to detect the position of the end of arm **110** in the external coordinate system, in accordance with movement of the arm in a y direction.

In one embodiment of the invention, spatial registration is used in combination with the system to record and monitor the three dimensional spatial position of the contact device **110** at all times, relative to a known reference point. One method of accomplishing the registration is through the use of a spatially encoded control arm **180**, which tracks the position of the contact device **110**. The control arm **180** holds the contact device **110** at one end, and is mechanically stabilized or fixed to the platform **620** at the other end. The control arm **180** engages drive mechanism **600**, allowing at one degree of freedom and up to three or more degrees of freedom, and may employ encoding devices to accurately determine the position and orientation of the contact device **110** relative to the

## 11

platform. The control arm **180** also allows movement and positioning of the contact device **110**. The control arm **180** is used to accurately and reproducibly position the contact device **110**. The positional information of the contact device **110** is then conveyed to localization software for registration of the position of the eye. The vertical or y position of the control arm can likewise be adjusted through movement of a drive **615** on which drive mechanism **600** is movably mounted, allowing both the x and y position of the control arm, and the eye-contact device attached to the control arm, to be accurately determined in the external coordinate system. In particular, the system functions to move the control arm to place the eye-contact device at a desired orientation, by the mechanism shown in FIGS. **8A** and **8B**, and then determine the position of the eye-contact device at this orientation from the known arm coordinates.

As will be discussed further below, the motion arm includes a biasing mechanism or element, such as a spring or magnetic element, that operates to bias the arm and an eye-contact device supported at the end of the arm against the patient. The biasing element, which is represented by force arrow **119** in FIGS. **2B**, **6A-6C** and **8A** and **8B**, may be a coil spring within or attached to mechanism **60** or a magnetic biasing mechanism, such as an electromagnetic mechanism that swings the arm in the direction of the patient with a desired biasing force of preferably between 1-25 grams, typically 5-20 grams. This mechanism for securing the contact device to the eye and stabilized the position of the eye is discussed below with reference to FIGS. **8A** and **8B**.

In a second and related general embodiment, the eye-contact device is equipped with a plurality of position indicators that are capable, in combination with detectors located in the external coordinate system, to locate the position of the contact device in the external coordinate system. This type of tool-tracking system, has been described for use in image guided surgery, where it is necessary to place a movable surgical tool, and typically also pre-op patient images, in a common surgical frame of reference containing the patient. In the present application, the position indicators may be three or more beam-directing elements designed to reflect external positioning beams, e.g., microwave beams from known-position beam sources to known-position beam detectors, with the position of the contact device being determined by a processor operatively linked to the beam detectors. Alternatively, the beam-directing elements in the eye-contact device can be equipped with a plurality of LEDs mounted on the device for directing, for example, a plurality of beams at known-position detectors to determine the position coordinates of the contact device in the external coordinate system. Such tool registration systems have been described, for example, in U.S. Pat. Nos. 7,139,601, 7,302,288, and 7,314,430, all of which are incorporated herein by reference in their entirety.

In a third general embodiment the position-determining means takes the form of a collimated light-beam assembly, including a laser light source and one or more optical components, such as a half-silvered mirror, for aligning the laser beam with the collimated irradiation beam produced by beam source **160**; such that the two beams are essentially coincident, along the same axis **168**. In this embodiment, the beam-positioning assembly is moved with respect to the patient's eye until the laser beam is aimed directly onto the selected target region of the patient's eye, e.g., the macula region at the central rear portion of the retina. As can be appreciated, this will place the selected target region of the eye in registry with the therapeutic irradiation-beam; that is, the laser beam acts

## 12

as a reference beam that functions to place the eye in the same frame of reference (coordinate system) as the irradiation beam.

More generally, the spatial registration and guidance of the contact device **110** may be through optical or electromagnetic sensor detection. In general, cameras or other detectors are mounted either on the system, or optionally in the treatment room, and are used to track and register the position of the eye or contact device **110**. Cameras or detectors are then able to determine and record the three dimensional position of the contact device **110** in real time, and therefore the position of the eye as it is positioned. A calibration process can be used to determine the relative spatial position of the contact device to a known reference frame, as well as in combination with optional images. The calibration information can be stored in a reference file on the computer and used by a software program.

With continued reference to FIG. **1**, system **100** also includes a processor or control unit **115** which has a graphical user interface **117** for receiving instructions from, and presenting information such as alignment and system functionality data to, a system operator. Further, the control unit **115** is in electronic communication with one or more of the other components of system **100** described above, e.g., the motors controlling the beam-positioning assembly, the motors controlling the eye-positioning assembly, and sensors, detectors and beam sources for determining the position of the eye-contact device in the external coordinate system, as described above. An electrical cable may be used to connect control unit **115** to the additional components. Alternatively, the connection between the control unit **115** to one or more of the components of the system is wireless.

Referring now to FIGS. **2A-2B**, top-down views of the contact device **110** being reversibly and controllably coupled to the cornea **200** and/or limbus and/or sclera **239** of the eye **130** is schematically illustrated. The eye **130** includes a cornea **200** and a lens **132** posterior to the cornea **200**. The eye **130** also includes a retina **134**, which lines the interior of the rear surface of the eye **130**. The retina **200** includes a highly sensitive region, known as the macula, where signals are received and transmitted to the visual centers of the brain via the optic nerve **136**. The retina **200** also includes a point with particularly high sensitivity known as the fovea. The eye **130** also includes a ring of pigmented tissue known as the iris **138**. The iris **138** includes smooth muscle for controlling and regulating the size of an opening in the iris **138**, which is known as the pupil. The eye **130** resides in an eye socket **140** in the skull and is able to rotate therein about a center of rotation.

The eye-contact device **110** functions to stabilize the eye in a first position to provide interactive support (e.g. stabilization and/or controllable movement) for the eye while the eye is being treated. The contact device **110** includes a cup or eye-contact member **120** which contacts eye **130**. The contact member **120** can be positioned on the eye in a variety of positions, and is therefore useful in a wide variety of ocular treatment procedures. In one embodiment, the eye-contact member is in at least partial contact with the cornea **200**. In a preferred embodiment, as illustrated in FIG. **2B**, the eye-contact member substantially covers but not necessarily touches the cornea of the eye **130** when in operative position. In a related embodiment, the eye-contact member substantially covers the cornea, but only makes contact with the limbus of the eye on the periphery of the eye-contact member **120**, such that the cornea is covered, but is not in direct physical contact with the surface of eye-contact member **120**. The contact member **120** is preferably a curved structure that

is substantially centered on the axis **235** with the periphery **237** of the contact member **120** in contact with the sclera **239** and overlying the cornea **200**. Thus, the curved contact member **120** is positioned to create an interior cavity between itself and the cornea.

The curved contact member **120** is preferably shaped with a concave eye-contact surface that will substantially conform to the anterior surface of the cornea **200** of the eye **130**. The contact surface of the contact member **120** preferably has a radius of curvature that is greater than about 5 mm. In one embodiment of the invention, the radius of curvature of the inner surface of the eye-contact member **120** is 7.38 mm. Likewise, in a preferred embodiment, the radius of curvature of the outer surface of the eye-contact member **120** is preferably 7.38 mm. It will be appreciated that a 1:1 ratio of inner and outer curvatures minimizes or eliminates refraction of energy through the eye-contact member **120** in certain embodiments of the invention; in this embodiment, the contact member **120** is a simple cup for the eye **130**. Alternatively, the inner and outer curvatures may differ to permit desired focusing or diffraction of energy as it is transmitted through the eye-contact member **120**. In some embodiments, the contact member **120** is produced in a variety of shapes, one or more of which can be chosen for a given patient depending on his or her specific anatomy.

As contemplated by the present invention, the eye-contact member **120** can be made of a number of materials well known in the art. In an exemplary embodiment of the invention, the contact member **120** is made from poly(methylmethacrylate), or PMMA. A certain degree of rigidity, or hardness, of eye-contact member **120** is of use in physically coupling with the eye and with the pivot which attaches to the control arm as described in further detail below. However, the eye-contact member **120** includes, in certain embodiments, a certain degree of flexibility, or softness, such that the eye-contact member **120** has a degree of flexibility, but still retains an arcuate shape in its resting position. In some embodiments, eye-contact member can break away from the contact device at a predetermined position along connector **222**, as described in greater detail below.

Preferably, the eye-contact member can be fashioned from any suitable material with attention to biocompatibility. Thermoset and/or thermoplast PMMA are contemplated by the present invention and are supplied by a number of sources, such as Perspex CQ (ICI Derby, England). Teflon and tantalum are also noted. It is also possible to coat eye-contact member **120** with biocompatible materials if elements of the eye-contact member **120** are not biocompatible. In some embodiments, the eye-contact member **120** contains pigments or dyes. In particular embodiments, the eye-contact member **120** is coated or impregnated with bioactive substances including anti-inflammatory agents/immunomodulating agents and/or anti-infective agents. Particular eye-contact members will contain radiopaque, radioactive, fluorescent, NMR contrast or other reporter materials.

With continued reference to FIGS. **2A** and **2B**, the contact member forms, with a back plate **121** of the contact device, an internal reservoir **122** by which a negative pressure (partial vacuum) applied to the device, through a vacuum port **210**, is distributed across the contact surface of the device, as can be appreciated. The vacuum port is connected to a suitable vacuum source through a tube **275**. In the embodiment illustrated in FIGS. **2A** and **2B**, the vacuum port **210** is positioned through the eye-contact member **120** such that an air or fluid communication space is formed through eye-contact member **120** to allow air trapped between eye-contact member **120** and the anterior surface of the cornea **200** of eye **130** to be

reversibly removed, thereby reversibly engaging the eye-contact member **120** with the anterior surface of the cornea **200**. In an alternative embodiment not shown, vacuum port **210** is attached to connector **270** which can contain a hollow lumen along axis **235** through eye-contact member **120** such that air between eye-contact member **120** and the anterior surface of the cornea **200** is capable of being reversibly removed as described above. Vacuum or suction assistance is useful for locating and adhering the scleral lens base on the eye **130** of the subject and securing the contact device **110** to the subject's eye **130**. Once in a desired treatment position, the contact device **110** can couple with the system **100** during the treatment procedure, as described below. Following treatment, the contact device **110** can be decoupled from the system **110** and removed from the subject.

In one preferred embodiment, negative pressure applied to the eye, for example, a negative pressure of 20-50 mm Hg, is effective to stabilize the position of the eye on the device, that is, substantially prevent movement of the eye with respect to the device, but by itself is not sufficient to hold the eye-contact device on the eye. Rather, the contact device is secured to the eye by a biasing force acting to bias the device against the patient's eye, acting in combination with the negative pressure applied to the eye by the device. In the embodiment illustrated, the contact device is secured to the eye by the biasing force acting through arm **180**, where the negative pressure applied to the contact device functions to prevent the eye from moving with respect to the device. As noted above, the contact device is typically biased against the eye with a force of between about 1-25, typically 5-25 grams, by a biasing spring, electromagnetic force, or the like. The advantage of this system is that the negative pressure applied to the eye can be substantially less than that which would be required if the vacuum alone were acting to hold the device to the eye, and this substantially lower negative pressure increases comfort and reduces irritation and deformation of the front portion of the eye. The biasing force is illustrated in the figures, e.g., FIG. **2B**, by an arrow **119**, which indicates the direction of action of the force in the figures.

When the eye-contact member **120** contacts eye **130**, negative pressure is applied to remove air from between the eye and contact member, to stabilize the position the eye **130** with respect to the contact member. A primary vacuum fitting is in fluid communication with the air passage. A vacuum line **275** is connected to the vacuum port **210**. Additionally, a vacuum pump is in air or fluid communication with the vacuum line **275** for evacuating the air trapped between eye-contact member **120** and the corneal surface **200**. Collectively, the vacuum port **210**, line **275**, and pump (not shown) constitute a primary vacuum subsystem. The degree of strength of the vacuum required to seal can be varied, and preferably controllably and continuously monitored, by the system of the invention. In one embodiment of the invention, between about 0.5 mm Hg and about 50 mm Hg are utilized to provide the negative pressure effective to stabilize the position of the eye with respect to the contact member **120**. Preferably, the vacuum is between about 20 mm Hg and about 50 mm Hg. More preferably, the vacuum force applied is about 25 mm Hg and is monitored by pressure sensors and/or by directly monitoring the vacuum source. In some embodiments, the pressure is held passively, for example, by a bladder. The bladder can be produced such that it can apply a given maximum pressure.

In one embodiment of the invention, one or more pressure sensors are placed onto the contact surface of eye-contact member **120** such that the pressure of the force being applied by the vacuum, and causing contact between eye-contact member **120** and the corneal surface **200** can be monitored

15

and selectively adjusted. The adjustment of the pressure can be automated. Throughout the treatment procedure, e.g., radiotherapy treatment, data from the pressure sensors can communicate to the control unit **115** via a communication link **185**. During the treatment and positioning procedure as illustrated in FIGS. 7A-7C, and discussed in detail below, the interactive forces that are generated between the eye-contact member **120** and the drive mechanism used to moveably rotate the eye can be monitored by pressure sensors. The force magnitudes experienced by the pressure sensors, and the differentials between the force magnitude, can be used to determine the magnitude and direction of the forces exerted against the eye **130** during the positioning and/or treatment procedures. In this way, the operation of the system **100** is monitored to ensure eye safety, and to minimize the risk of unwanted damage or injury to the eye **130**. Specifically, whenever a predetermined force threshold is reached, either in the direction or the magnitude of the forces exerted on the eye **130**, further movement of the subject's eye is prevented by the control unit **115**.

When activated, the primary vacuum subsystem evacuates air through vacuum port **210**. The evacuation of air creates a negative pressure at the interface of the eye-contact member **120** and the anterior surface of the cornea **200** and/or sclera. The present invention also contemplates use of one or more sensors to detect whether a vacuum is formed. In the event the eye-contact member is not properly seated on the eye **130**, the partial vacuum will not form. In this case, an error message is displayed for the system operator on the graphical user interface **117** of the control unit **115** of FIG. 1. The error message may be an audio message, a visual message, or a combination of the two. In one embodiment of the invention, suction is used to initially engage the contact device **110** to the eye **130**, and following initial engagement, the suction is removed and the contact device **110** remains on the eye throughout the treatment procedure. In another embodiment of the invention, suction is used to initially engage the contact device **110** to the eye **130**, and following initial engagement, the suction force is maintained throughout the treatment procedure.

By engaging the contact member **120** with the eye **130**, the eye **130** becomes fixed in a first position, the patient unable to move the contact member with intra-ocular movements. The contact member can, however, be moved using control arm **180**; the movement by the control arm rotates the eye through the eye-contact member. Thus, one embodiment of the invention includes substantially stabilizing the eye **130** in a selected position with the eye-contact member **120**.

With continued reference to FIGS. 2A and 2B, contact device **110** also includes a pivot joint or connector **220** which accommodates pivot movement between the contact member and positioning arm **180**, as the arm moves the contact device to a desired orientation in the external coordinate system. In a preferred embodiment, pivotable connector **220** is a spherical or ball pivot joint which allows rotation in three dimensions. As seen best in FIGS. 3A and 3B, positioning arm **180** may be releasably coupled to the contact device through a stem-and-socket arrangement which fastens the end of arm **180** to a socket formed in ball joint **220**.

Eye-contact member **110** also includes a beam-directing mirror **230** or other detector or sensor, which in combination with the laser system **150**, allows the position and rotation of the eye to be placed at a desired orientation or position in the external coordinate system. As shown, the mirror **230** is parallel to the eye-contact member **120** and provides a reflective surface to align the contact device **110** to the eye and to the treatment device. The position of the mirror **230** also provides a known reference to the subject's corneal apex by virtue of

16

the contact member fitting closely to the eye upon application of some vacuum. The alignment of the eye-contact member with a reference laser beam will be described below with reference to FIGS. 8A and 8B.

In one embodiment, the mirror **230** includes a reflective material that reflects at least one wavelength of light. In some embodiments, the characteristic of a treatment device **160**, e.g., a radiation beam, is determined by the information and includes at least one of a trajectory of the radiation beam and an emit/not-emit status. In some embodiments, the communication link to the treatment device **160** is an optical link. In some embodiments, the contact device **110** is adapted to align the treatment device **160** with a visual axis of the eye. Some embodiments further include a camera that visualizes a position of the eye relative to the contact device **110**. In some embodiments, the camera detects movement of the eye and communicates data relating to the eye's movement with imaging software.

In other embodiment, the eye-contact device includes a plurality of fiducials and/or a plurality or beam-directing elements by which the position of the eye-contact member, and thus the position of a patient eye stabilized in the contact member, in an external coordinate system can be determined. As noted below, multiple fiducial arrays or multiple beam-directing arrays may be monitored by camera or beam-sensing detectors for determining the position of the fiducial or beam-directing elements in the external coordinate system.

In some embodiments, the eye-contact member **110** is attachable to a surface external to the eye. In some embodiments, the eye-contact member **110** is mechanically linked to a eye-position assembly that includes control arm **180**. In some embodiments, the contact device **110** is engaged with the eye **130** by docking the contact device **110** into position on the eye **130** (e.g., by the physician) so that the center of the holder has a center in common with the limbus of the eye. This common center is a step in assuring that the treatment device is aligned with the optical or geometric axis of the eye. With knowledge of the center of the limbus in combination with an eye model, the treatment device **160** can then be directed about a treatment axis and center of the limbus to deliver treatment, e.g., radiation, to a target region of the eye, e.g., the retina. The position of the eye **130** can also be tracked by a treatment system **160**, e.g., a radiotherapy system.

Some embodiments further include a material that is transmissive of energy through the contact device **110**. In some embodiments, the radiation beam comprises laser light. In some embodiments, the radiation beam comprises x-rays. Some embodiments further include a material that is transmissive of energy through at least a portion of the contact device **110**. Energy sources contemplated by the present invention include radio waves, microwaves, infrared light, visible light, ultraviolet light, x-rays and gamma rays.

In some embodiments, the energy comprises laser light. In some embodiments, the energy comprises x-rays. In an alternative embodiment, the energy comprises protons for use in proton therapy or gamma rays for use in gamma ray therapy. In some embodiments, the eye-contact member **120** includes a transmissive portion that transmits a first wavelength of electromagnetic radiation from outside to inside the eye.

In some embodiments, the first portion is reflective of a second wavelength of electromagnetic radiation. Thus, the eye-contact member **120** may selectively allow transmission of one or more preferred wavelengths of electromagnetic radiation. Eye-contact member **120** may selectively reflect one or more wavelengths of electromagnetic radiation. In one embodiment of the invention, eye-contact member **120** selectively allows transmission of one or more preferred first

wavelengths of electromagnetic radiation, and also selectively reflects one or more second wavelengths of electromagnetic radiation. In one embodiment, the portion selectively reflecting and/or selectively transmitting one or more wavelengths of electromagnetic radiation is centrally located in the eye-contact member **120**. In another embodiment, the portion selectively reflecting and/or selectively transmitting one or more wavelengths of electromagnetic radiation is off-centered, on the eye-contact member. In one embodiment, the portion selectively reflecting and/or selectively transmitting one or more wavelengths of electromagnetic radiation is peripherally located in and/or on the eye-contact member **120**. In some embodiments, at least one of the plurality of wavelengths of electromagnetic radiation comprises laser light beams. In some embodiments, at least one of the plurality of wavelengths of electromagnetic radiation comprises x-ray beams.

FIG. **3A** is a side view of contact device **110** illustrating the pivotability of control arm **180** around the spherical pivotable connector **220**. The control arm/contact device assembly includes a swiveling tiltable head **190** carrying a conical divot or the like providing a good mating fit. In the embodiment shown, the head **190** of control arm **180** is tilted with respect to a spherical coupling **220** positioned within the conical divot of head **190**. The coupling includes a hollow interior within control head **190** that is located at the end of control arm **180** or other connector that snap-fits onto and rotatably rides upon a mating connector **220**. In one embodiment of the invention, the swiveling head **190** is designed to coincide with the center of mass of the contact device. The swiveling and tiltable head **190** permits a wide range of motion of the eye-contact member **120** when the spherical pivot is inserted into the hollow interior of head **190** of control arm **180**. Thus, movement of the control arm **180** in the X, Y, and/or Z directions as illustrated in FIG. **3A**, permits the contact device to be controllably positioned. Importantly, when the contact member **120** and holder are fixed with vacuum to the eye as shown in FIG. **2**, a greater degree of friction is created between the spherical pivot **220** and the head **190** of control arm **180** so that the eye moves very little after vacuum is applied. Moreover, the eye pivots around a point toward its posterior as it is pulled by intraocular muscles which rotate the eye around this posterior point. When the eye-contact member is coupled to the eye, the eye and the holder are locked together at the pivot point of each. The intra-ocular muscles cannot move the contact member around its pivot which is the only way the contact member can move. Arm **180** can move contact member **120** through spherical bearing **220**. Similarly the patient's face or head can move the contact member by translation of their head or body which would similarly induce a movement about spherical pivot **220**. However, the muscles of the eye cannot move contact member **120** when it and the eye are held together. As a result of such rotational articulation and subsequent coupling, including the friction between the hollow interior of head **190** and spherical pivotable connector **220**, the contact device **120** can be positioned on an eye and stabilized. Such rotational positioning of the contact device and coupling of the pivot points also allows the mirror **230** of the contact device to be aimed or aligned with the system within a known coordinate system.

The friction between head member **190** and pivotable connector **220** can be increased or decreased as desired by varying the surface of the pivotable connector **220** and/or head member **190**. For example, to decrease the friction between the pivotable connector **220** and the head member **190**, a metal may be used which can be electropolished by a predetermined amount to provide the desired extent of smoothness.

Alternatively, one or both of the surfaces of pivotable connector **220** and head member **190** may be dimpled on either a micro or macro level using known surface finishing or machining techniques to increase or decrease friction accordingly. Additionally, a liquid lubricant, such as glycerin can be applied to the surface of the pivotable connector **220** to reduce the friction at the head member **190**/pivotable connector **220** interface, as desired.

Distal end of the control arm **180** has little or no free movement as its x-y position is controlled manually or automatically. However, once the holder and the eye are coupled to one another, the eye can be positioned by positioning the arm **180** in the X-Y directions or positioning the patient's head. Arm **180** can have some flexibility in the Z direction, acting as a cantilever, so that the holder **120** on the eye is not completely rigid. Alternatively, a mechanism is provided which controllably adjusts the contact member in the z direction.

FIG. **3B** is a perspective view of contact device **310** showing a straight control arm **380** for mechanically linking contact device **310** to a system for controllably positioning an eye for treatment. In one embodiment, the eye-contact surface of eye-contact member **120** contacts the sclera of eye **130**. In another embodiment, the eye-contact surface contacts the cornea of eye **130**. In yet another embodiment, the eye-contact surface of eye-contact member **120** is in contact with both the cornea and the sclera. In some embodiments, the contact device **110** includes a portion which is at least partially opaque or reflective to x-ray energy. In some embodiments, the eye-contact holder **110** includes at least a portion that is at least partially transparent to x-ray energy. In some embodiments, the contact device **110** is configured to apply a suction to the eye **130** through vacuum port **210**. Some embodiments further include a contact device **110** that is configured to contact the eye **130** and maintain a position of the eye. In the embodiment of the invention illustrated in FIG. **3B**, the control arm **180** is generally cylindrical. As used herein, the term "generally cylindrical" is not limited to a perfectly cylindrical surface, but instead is understood to include any faceted or other column or like structure (e.g., an octagonal cylinder, a hexagonal cylinder, etc.). The material strength of the arm is controllable such that a thin arm has greater spring than a thick arm. The thicker arm can therefore apply greater force to the eye when the subject is positioned in the holder **120**. In some embodiments of the invention a strain gauge is used to measure the resistance and/or change in resistance as the control arm **180** is deflected during positioning and/or stabilization of the contact device **110**.

FIGS. **3C** and **3D** illustrate alternative embodiments of contact devices **312** pivotably connected to control arms **180** and **380**, respectively. As can be seen in FIG. **3C**, eye-contact member **320** is connected to spherical pivot **220** through connector **302** off-center of contact member **320**. In the embodiment shown, the head **190** of control arm **180** is tilted with respect to a spherical coupling **220** positioned within the conical divot of head **190**. The coupling includes a hollow interior within control head **190** that is located at the end of control arm **180** or other connector that snap-fits onto and rotatably rides upon a mating connector **220**. Vacuum port **304** is in air or fluid communication with connector **302** which is in air or fluid communication with a space formed through eye-contact member **320** which is in air or fluid communication at the eye/contact device interface when the contact device **312** is positioned on the eye of a subject.

FIG. **4** illustrates an exploded view of the contact device **110** with each component of one embodiment of the contact device **110** separated. Eye-contact member **120** can be revers-

ibly coupled to pivotable connector **220** at coupling points **224**, **226** which can be reversibly coupled to mirror **230** at coupling points **228**, **229**. Such coupling may include interlocking snaps, glue, welding, magnets, etc. The mirror can be painted, sprayed or applied with a vacuum deposition process. The coupling preferably includes one or more magnets, as illustrated in FIGS. **4B-4C**.

More generally, FIGS. **4B** and **4C** and **4D** and **4E** illustrate two embodiments of an eye contact device in accordance with one aspect of the invention in which an eye-contact member is releasably coupled to a positioning arm through releasable coupling members carried on each component of the assembly. In FIGS. **4B** and **4C**, the assembly is indicated at **422** and includes an eye-contact member **120** having a first magnet **410** thereon, and an arm-attachment member **190** carrying a second magnet **415** thereon. As seen in FIG. **4C**, as the first coupling member **415** is brought toward the second coupling member **410**, the two coupling members couple the eye-contact member **120** with the spherical pivot **220** which mates with the head **190** of control arm **180** such that the eye-contact member **120** is connected to the system. This allows the eye-contact member **120** to move together with control arm **180** and therefore be in a known position within the coordinates of the system. Thus, in operation, the eye-contact member **120** may be positioned on the eye of a subject prior to magnetically coupling the two coupling members **410**, **415**. In an alternative embodiment, the eye-contact member **120** is positioned on the eye of a subject following magnetically coupling the two coupling members **410**, **415**. The magnetic coupling can also be used as a safety feature in that the magnets become uncoupled when force is applied in a direction which is not co-linear with the perpendicular axis to the magnets.

In a similar manner, FIGS. **4D-4E** illustrate a snap fit coupling or mechanical coupling between the eye-contact member **120** and control arm **180** in a second embodiment of an eye-contact assembly **416**. In FIG. **4D** a snap or plurality of snaps is disposed on the first snap coupling member **417** for snap coupling with a snap or plurality of snaps on the second snap coupling receiving member **412**.

In the embodiment illustrated in FIGS. **4D-4E**, eye-contact member **120** is attached to second snap coupling receiving member **412**, which includes a built-in divot **420**. In this embodiment, the divot **420** includes a female receptacle, such as the illustrated conical depression. However, as used herein, a divot also refers to any other male or female receptacle, or the like. The divot **420** is capable of receiving a correspondingly sized and shaped mating tip **430** which is coupled to the first snap coupling member **417**, which is thereby coupled through spherical pivot **220** to control arm **180**. Such a control arm **180** is useful for registering the actual physical location of the subject's eye prior to, during, or following a selected treatment procedure. The registration can be accomplished using known coordinates within the system, or by obtaining images. Such images are typically stored in memory of an image-guided treatment computer workstation.

As seen in FIG. **4E**, as the first snap coupling member **417** is brought toward the second snap coupling receiving member **412**, the two coupling members couple the eye-contact member **120** with the spherical pivot **220** which mates with the head **190** of control arm **180** such that the eye-contact member is connected to the system. This allows the eye-contact member **120** to move together with control arm **180** and therefore be in a known position within the coordinates of the system. Thus, in operation, the eye-contact member **120** may be positioned on the eye of a subject prior to snap coupling the two coupling members **410**, **415**. In an alterna-

tive embodiment, the eye-contact member **120** is positioned on the eye of a subject following magnetically coupling the two coupling members **410**, **415**. That is, the releasable coupling members in the assembly are deformable, typically plastic, members with complementary interlocking shapes.

The snap fit or magnetic fit is not only of structural importance but can provide for an emergency breakaway mechanism if the subject's eye needs to move out of the restraint system shown in FIG. **1**, as described in detail below. In a preferred embodiment, the releasable coupling members couple the eye-contact member to the arm with a release force sufficient to allow the device and a patient eye stabilized therein to be moved by the arm, and to release from one another when an above-threshold force is applied to the eye, e.g., by sudden eye movement, or abrupt arm movement, so that the eye is protected from injury that could result from sudden relative movement between the eye and contact member. The release force, that is, the force required to release the two components, may be in the same range, but typically somewhat greater than the biasing force used in biasing the contact device against the patient's eye, e.g., in the range 10-100 grams.

In one embodiment of the invention, one or more pressure sensors are positioned on coupling member **410**, as illustrated in FIG. **4F**. When the control arm **180** is mechanically engaged with the eye-contact member **120**, the second magnetic coupling member **415** will contact one or more pressure sensors of which pressure sensors **450**, **452**, **454** are exemplary. Preferably, when in contact with second magnetic coupling member **415**, the pressure sensors **450**, **452**, **454** lie in a plane that is substantially parallel to the plane of the first magnetic coupling member **410**. As illustrated in FIG. **4F**, the pressure sensors **450**, **452**, **454** are each positioned an equal distance from the center point of the first magnetic coupling member **410**. Also shown in FIG. **4F** is the position of the pressure sensors **450**, **452**, **454** relative to each other. Specifically, the three pressure sensors **450**, **452**, **454** are equidistant from each other, i.e., positioned 120 degrees apart. In an alternative embodiment of the invention, a plurality of pressure sensors are positioned on the second magnet coupling member **415**.

In operation of this embodiment of the present invention including pressure sensors, once the eye-contact member **120** is positioned on the eye, and the control arm **180** is coupled to known coordinates within the system, the control arm **180** is moved through a "docking" procedure whereby the control arm **180** is moved to engage with the eye-contact member **120**. During this docking procedure, the two magnetic coupling members **410**, **415** are engaged. As intended by the present invention, the two magnetic coupling members **410**, **415** are dimensioned to precisely match and reversibly couple to each other with the pressure sensors positioned therebetween. During the docking procedure, the interactive forces that are generated between the control arm **180** and the eye-contact member **120** are monitored by the pressure sensors **450**, **452**, **454**. It can be appreciated by those skilled in the art that the force magnitudes experienced by the pressure sensors **450**, **452**, **454**, and the differentials between the force magnitudes, can be used to determine the magnitude and direction of the forces exerted against the eye during the docking procedure. In this way, the operation of the system is monitored to ensure patient safety, and to minimize the risk of unwanted damage to the eye. Specifically, whenever a predetermined force threshold is reached, either in the direction or the magnitude of the forces exerted on the eye, further movement of the control arm **180** toward the eye-contact member **120** is prevented by the control unit. In one embodiment, when the

threshold force is reached, the control arm **180** can only be moved in a direction away from the eye-contact member **120**.

In yet another embodiment, when a predetermined force threshold is reached during the docking procedure or during treatment, such as when the subject moves out of position, the eye-contact member **120** can break away from control arm **180** such that patient safety is ensured. In this embodiment of the invention, if the interactive forces that are generated between the control arm **180** and the eye-contact member **120** reach a predetermined level, the magnetics or snaps may be controllably decoupled to permit the contact device **120** to break away or disengage from control arm **180**. Simultaneously, when a predetermined level of interactive force or magnitude is reached, and the contact device **120** is disengaged from the control arm **180**, the treatment or diagnostic procedure may be terminated.

In a similar manner, in accordance with another embodiment of the invention, when the control arm **180** is used to positionably rotate the eye in a controlled manner, pressure sensors **450**, **452**, **454** monitor the interactive forces that are generated between the control arm **180** and the eye-contact member **120**. The force magnitudes experienced by the pressure sensors **450**, **452**, **454**, and the differentials between the force magnitudes, can be used to determine the magnitude and direction of the forces exerted against the eye during the positioning procedure. In this way, the operation of the system is dynamically monitored to ensure patient safety and to minimize the risk of unwanted damage to the eye throughout the eye positioning and stabilization procedure. Specifically, whenever a predetermined force threshold is reached, either in the direction or the magnitude of the forces exerted on the eye, further movement of the control arm **180** is prevented by the control unit. In a related embodiment, whenever a predetermined force threshold is reached, further movement of the control arm **180** is prevented by the control unit, and the coupling, e.g., snap or magnetic coupling, between the control arm **180** and the contact device **120** is disengaged, decoupled or permitted to break away to ensure patient safety.

In one embodiment of the invention, when the predetermined force threshold described above is reached, the magnetic field between the two magnetic coupling members **410**, **415** is turned off to allow the eye-contact member **120** to decouple from the control arm **180**. In another embodiment, the treatment system is turned off when the predetermined force threshold described above is reached. In yet another embodiment, when the predetermined force threshold described above is reached, the magnetic field between the two magnetic coupling members **410**, **415** is turned off to allow the eye-contact member to decouple from the control arm **180**, and the treatment system **160** is turned off or prevented from being turned on such that the safety of the eye is continuously monitored and dynamically maintained throughout the eye positioning and/or treatment procedures.

In one embodiment the entire contact device **110** is molded as a single component. The contact device **110** includes, in one embodiment, an optical or other communication between the system **100** and the eye **130** by inhibiting movement of the subject. The contact device contains, in some embodiments, one or more of a radiotransmitter, a laser pointer, and/or features which can be captured on a camera so that the eye can be located in three-dimensional space.

Referring again to FIG. **4A**, the contact device **110** contains, in some embodiments, a mirror **230**. The mirror **230** can function as a beam reflector to indicate alignment or misalignment of the laser device **150** and/or the treatment device **160**, e.g., a radiotherapy device. As the contact device **110** is positioned in contact with the eye, a proper engagement and

alignment between the contact device **110** and the system is achieved. To this end, the laser light source **150** that is mounted on the platform is used to verify and monitor proper alignment. The light emanating from the light source is used to create a pattern of reflected light that is observable by the system operator, or in some embodiments, by an automated system. Referring now to FIGS. **8A-8B**, an exemplary path of reflected light **830** is shown relative to the path of the source light **810**. Importantly, when the pattern of reflected light **830** is reflected directly back along the path of the source light **810**, the contact device **110** is properly engaged and aligned with the system. If, however, the contact device **110** is not properly or fully aligned with the laser **800**, the path of reflected light **830** will be displaced or distorted from its preferred orientation. In this situation, as shown in FIG. **8A**, the path of reflected light **830** relative to the path of the source light **810** emanating from the distal end **820** of laser **800** is indicative of an improper alignment. Further, the system operator can observe the misaligned path of reflected light directly, or on the graphical user interface, and properly align the contact device **110**.

For example, the mirror **230** will reflect a light such as a laser pointer or an LED. The light originates on the laser device **800** and/or treatment device, and its reflection from the mirror **230** is indicative of the direction of the mirror relative to the laser device **800** and/or treatment device. The mirror **230** can be parallel to the surface of the cornea, and therefore, a beam perpendicular to the mirror is approximately perpendicular to the cornea. If a lumen, such as the lumen **250** as shown in FIGS. **4B-4F** through the center of the mirror is present, and the eye-contact member **120** is transmissive of light at its center, a perpendicular beam to the cornea will travel through the optical or geometric axis of the eye and reach the center of the posterior pole of the eye. The lumen notwithstanding, the beam being reflected from the mirror **230**, also represents the optical axis of the eye.

In some embodiments, the mirror **230** is a so-called "hot mirror" or a "cold mirror" in which the mirror **230** reflects some wavelengths and transmits others. For example, a "hot mirror" can reflect an infrared laser pointer and transmit visible light so that the patient or treating physician or a camera will be able to see through the lens. A "cold mirror" will transmit infrared and reflect visible so that a visible laser pointer can be reflected while infrared can be transmitted; cold mirrors can be used, for example, in cases where it is desired to utilize an infrared fundus camera during treatment.

As noted above, in some embodiments, contact device **110** can include material that is radiotranslucent, or that permits at least some radiation to pass. In some embodiments, the radiotranslucent material of the coupling device can be configured to permit the passage of the therapeutic x-ray beams during treatment. For example, the contact device can engage the eye to maintain position of the eye, and the x-ray beams can be directed to target eye tissue with a trajectory that passes through at least a portion of the contact device **110**. Accordingly, a treatment planning system can plan x-ray beam trajectories without significant consideration of where the contact device engages or is positioned on the eye.

In some embodiments, the contact device **110** can include material that is radiopaque, or that reduces or limits the transmission of radiation. In some embodiments, the radiopaque material of the contact device **110** can be configured to limit transmission through the material of radiation, such as, for example, x-ray beams. For example, the contact device **110** can engage the eye to maintain position of the eye, and x-ray beams that are directed to target tissue of the eye will not be permitted to pass through, or transmission of the x-ray beams

through the material will be substantially limited, the contact device **110**. In these embodiments, the contact device **110** can be used as a shield for critical structures of the eye (e.g., the lens, the optic nerve, the cornea, and so forth) by limiting radiation exposure to these structures.

FIGS. **5A-5B** are perspective and enlarged views of contact device **110** showing a preferred embodiment of the contact device **110** including the contact member **120**, spherical pivot **220**, mirror **230** and vacuum port **210**. In this embodiment of the invention, the contact device **110** includes one or more fiducial markers **240**, **242**, **244**, **246**, **248** which define the geometry of the contact device **110** or geometric relationships between the contact device **110** and additional components of the system and/or eye as described throughout the specification. The fiducial markers, in one embodiment of the invention, contribute to the positional knowledge of the eye when the contact device **110** is engaged with the eye **130**, and a coordinate system is known. Spatial registration can be used record and monitor the three dimensional spatial position of the contact device **110** relative to a known reference point.

In the embodiment illustrated in FIGS. **5A-5B**, one or more of the fiducial markers **240**, **242**, **244**, **246**, **248** includes an imageable fiducial locator. The fiducial locator is locatable using one or more imaging system modalities. In this embodiment, the fiducial is capable of being mounted in or on the eye-contact member **120**, such as being either flush to, or recessed from, an outer surface of eye-contact member **120**. However, in alternative embodiments, the fiducial need not be configured for mounting flush to or recessed from contact member **120**, and can be mounted to extend from eye-contact member **120**. In another embodiment, one or more fiducials are positioned on, within, or on the perimeter of mirror **230**. This allows the mirror **230**, along with contact device **110**, to be centered or aligned with respect to the limbus or other ocular structure.

The fiducial may include a liquid or gel housed in a sealed interior cavity. Preferably, the fiducial is a solid. The solid, gel, or fluid may be visible by one or more imaging modalities (e.g., MR, CT, etc.). In one embodiment, the fiducial is integrated into the eye-contact member itself. The imaging fiducial is visible and provides good contrast on images produced by at least one imaging modality. In one embodiment, the imaging fiducial is multimodal (i.e., locatable by more than one imaging modality), such as by using a mixture of different imaging fluids, gels or solids that are locatable on different imaging modalities.

In one embodiment, the one or more of the fiducial markers **240**, **242**, **244** includes a substance that is viewable on a first imaging modality, while one or more of the fiducial markers **246**, **248** includes a substance that is viewable on a different second imaging modality. In one such illustrative embodiment, the one or more of the fiducial markers **240**, **242**, **244** includes, or is doped with, a substance having a high atomic number (*Z*), such as barium, titanium, iodine, gold, silver, platinum, stainless steel, titanium dioxide, etc. that provides good contrast on a CT or other radiographic imaging system. In this embodiment, one or more of the fiducial markers **246**, **248** include gadopentatate dimeglumine, gadoteridol, ferric chloride, copper sulfate, or any other suitable MRI contrast agent, such as described in chapter 14 of *Magnetic Resonance Imaging*, 2nd ed., edited by Stark and Bradley, 1992, which is incorporated herein by reference.

In an alternative multimodal embodiment, the fiducial marker is constructed of a substantially solid plastic or other material that is hygroscopic, i.e., capable of receiving and retaining a fluid, such as an imaging fluid that is viewable on an imaging system (e.g., an MRI imaging system or the like).

In a further embodiment, the plastic forming the fiducial marker is doped or otherwise includes a substance that is viewable on a different imaging system, such as, for example, a CT or other radiographic imaging system. Illustrative examples of solid plastics that can be made hygroscopic include, among other things, nylon and polyurethane. Using a hygroscopic material avoids the complexity and cost associated with manufacturing a sealed cavity for retaining an imaging fluid. Moreover, by adapting the solid hygroscopic plastic for imaging using a first modality, and by using the imaging fluid for imaging using a second modality, each of the solid and the fluid can be separately tailored toward providing better contrast for its particular imaging modality.

In a further embodiment of the fiducial markers illustrated in FIGS. **5A-5B**, the outer surface of one or more of the fiducial markers is reflective of light or other electromagnetic energy. Consequently, it is locatable by a camera in an optical positioning system that is coupled to an image-guided workstation (e.g., during subject registration). One additional function of such fiducials is measurement calibration where the distance between fiducials is used to calibrate distance on or within the eye. In one such example, the outer surface of the imaging spherical fiducial marker includes light-reflective microspheres (e.g., embedded in an adhesive covering the fiducial or eye-contact member **120**). In another such example, the outer surface of the fiducial is covered with an adhesive-backed light-reflective tape, such as SCOTCHLITE 9810 Reflective Material Multipurpose Tape sold by Minnesota Mining and Manufacturing Co. ("3M"), of Saint Paul, Minn.

In one embodiment of the invention, the spherical pivot **220**, mirror **230** and/or the control arm **180** includes one or more fiducial markers. In an alternative embodiment of the invention, the one or more fiducial markers are configured to be locatable by a remote positioning system as well as imageable using one or more imaging modalities. In one such embodiment, the outer surface of the eye-contact member is configured to be light reflective, such as discussed above. The fiducial markers are still advantageously locatable using one or more imaging modalities (e.g., MR, CT, or other imaging system providing 3D or other internal images within a subject) as well as also being locatable external to the subject, such as by using a remote camera or like component of an optical or other positioning system, e.g., that is coupled to an image-guided workstation. In one embodiment, this permits automatic registration of the actual location of the subject's eye (e.g., using cameras to locate the light reflective fiducial markers) to pretreatment images of the system on which additional imageable fiducial markers are positioned. This eliminates the need to register the eye of the subject by inserting an optically-locatable positioning control arm onto the contact device, and eliminates the need for other absolute position reference, because the fiducial markers themselves are optically locatable and registerable to known locations on pretreatment images of the system.

FIG. **5B** illustrates one embodiment of the control arm **180** coupled to contact device **110**. Control arm **180** is coupled to an image-guided workstation or platform (not shown). In this embodiment, control arm **180** includes an end that is sized and shaped to permit being coupled to spherical pivot **220**. The control arm **180** includes, in this embodiment, a plurality of fiducial markers **520**, **522**, **524**, **526**, **528**, **530** that are locatable by a camera or other like device of the optical positioning system. The fiducial markers **520**, **522**, **524**, **526**, **528**, **530** on the control arm **180** are positioned in a known spatial relationship to each other and to the tip of the control arm **180**. By recognizing the locations of the fiducial markers,



the optical positioning system is capable of computing the location of the control arm tip, which is in a known spatial relationship with the configuration of the fiducial markers. This permits the control arm **180** to be used in conjunction with the optical positioning system to register the eye of the subject and to further plan and/or perform the treatment procedure using an image-guided workstation. An image guided treatment computer workstation, which is capable of displaying previously acquired and loaded pretreatment images of a the system. The optical positioning system connected to the workstation includes an infrared light (or other energy source) that provides light that is reflected from the reflective fiducial markers. This permits the reflective fiducial markers on the control arm **180** to be located and recognized by the cameras.

As seen in FIGS. **5A-5B**, an additional component of the contact device **110**, in some embodiments and as discussed with reference to FIGS. **4B-4D** above, is a lumen **250** which traverses the contact device **110** and, in some embodiments, extends to the surface of the eye. The lumen **250** can be used to pass one or more probes such as may be used to determine the axial length of the eye (e.g., an A-scan). In some embodiments, the probe includes a laser pointer probe (not shown), which can point outward away from the eye of the subject. The outward pointing laser pointer can be used to determine alignment of the device, and therefore the eye, relative to a treatment device included within the system. In some embodiments, the laser pointer is used to align the treatment device with an axis of the eye and can be used to turn the treatment device on (when in position) or off (when not in position). In these embodiments, the subject turns the device on and off, and the treatment device operates when the eye is aligned with the machine and turns off when the device is not aligned with the radiotherapy device.

In some embodiments, the contact device **110** can include material that is radiotranslucent, or that permits at least some radiation to pass. In some embodiments, the radiotranslucent material of the contact device **110** can be configured to permit the passage of therapeutic radiation beams during treatment. For example, the contact device **110** can engage the eye to maintain position of the eye, and x-ray beams can be directed to target eye tissue with a trajectory that passes through at least a portion of the contact device **110**. Accordingly, a treatment planning system can plan x-ray beam trajectories without significant consideration of where the contact device **110** engages or is positioned on the eye.

In some embodiments, the contact device **110** can include both material that is radiopaque and material that is radiotranslucent. In some embodiments, the radiopaque material of the contact device **110** can be configured to limit transmission through the material of radiation, such as, for example, x-ray beams, and the radiotranslucent material can be configured to permit transmission of radiation (e.g., x-ray beams) to pass through the material. The contact device **110** can further be configured to provide alignment trajectories along which the x-ray beams will pass to the target tissue. In some embodiments, the contact device **110** can further operate as a tertiary collimator by limiting the beam size or shape. For example, the radiotranslucent material of the contact device **110** can be sized and shaped as the aperture through the secondary collimator. In such embodiments, when the x-ray beam is emitted through the radiotranslucent material, any penumbra at the contact device **110** can be blocked by the surrounding radiopaque material. In some embodiments, apertures in the radiopaque material may be provided instead of radiotranslucent materials. Accordingly, the contact device **110** can further provide shielding or targeting functions.

In some embodiments, the contact device **110** can have a radiopaque material that comprises substantially a central portion of the contact device **110** (e.g., a portion of the eye-contact member **120**), and a portion of the contact device **110** extending around a periphery, or the edges, of the central portion comprises radiotranslucent material. Accordingly, the central portion can operate as a shield to structures of the eye, and the x-ray beams can pass through the radiotranslucent material during radiotherapy. Thus, the contact device **110** can have a larger eye-contact member **120** to engage the eye while still permitting x-ray beams to reach the target tissues substantially unimpeded by the radiopaque material.

FIGS. **6A-6C** illustrate perspective views of the contact device **110** attached to control arm **180** which is being fed into slot **610** of drive mechanism **600**. In some embodiments, the contact device **110** of the system can be attached to a coupling component to hold the eye in place. The coupling component can be attached to the treatment device, but preferably, as shown in FIGS. **6A-6C**, it is attached at a location separate from the radiotherapy device, such as a drive mechanism **600** that is attached to a table or platform **620** which holds the treatment device. Contact device **110** is preferably disposable such that a separate (e.g. disposable) contact device **110** is employed for each subject and/or use. Alternatively, contact device **110** may be nondisposable and be treated, e.g., with anti-infective agents, prior to being utilized in multiple subjects' eyes. Drive mechanism **600** is fixed to base **620** through connector **640**, which is may robotically controlled, but preferably manually controlled, and has a known coordinate system. In one embodiment, drive mechanism **600** is fixed in a known, or predetermined, location with respect to the head positioning system (not shown) and/or the eye of the subject (not shown) and/or the positioning system of the radiotherapy device. Push button **630** allows free manual positioning of contact device **110** into and/or out of slot **610**. Thus, as illustrated in FIG. **6A**, the control arm **180** is not engaged with the drive mechanism **600**. In FIG. **6B**, the control arm **180** is partially engaged with the drive mechanism **600**. And in FIG. **6C**, the control arm **180** is fully engaged with the drive mechanism **600** and is fixed in a known, or predetermined location, which allows the eye of the subject to be fixed in a known, or predetermined location, when contact device **110** engages the eye.

In one embodiment of the invention, spatial registration is used in combination with the system to record and monitor the three dimensional spatial position of the contact device **110** at all times, relative to a known reference point. One method of accomplishing the registration is through the use of a spatially encoded control arm **180**, which tracks the position of the contact device **110**. The control arm **180** holds the contact device **110** at one end, and is mechanically stabilized or fixed to the platform **620** at the other end. The control arm **180** engages drive mechanism **600**, allowing at one degree of freedom and up to three or more degrees of freedom, and may employ encoding devices to accurately determine the position and orientation of the contact device **110** relative to the platform. The control arm **180** also allows movement and positioning of the contact device **110**. The control arm **180** is used to accurately and reproducibly position the contact device **110**. The positional information of the contact device **110** is then conveyed to localization software for registration of the position of the eye.

Another method to accomplish the spatial registration and guidance of the contact device **110** is through optical or electromagnetic sensor detection. In this technique, cameras or other concentrated detectors are mounted either on the system, or optionally in the treatment room, and are used to

track and register the position of the eye or contact device **110**. Cameras or detectors are then able to determine and record the three dimensional position of the contact device **110** in real time, and therefore the position of the eye as it is positioned. A calibration process can be used to determine the relative spatial position of the contact device to a known reference frame, as well as in combination with optional images. The calibration information can be stored in a reference file on the computer and used by a software program.

FIGS. 7A-7C illustrate a preferred eye stabilizing and positioning embodiment of the invention. In FIG. 7A, contact device **110** is moved toward eye **130** along directional arrows **710**, **712** such that eye-contact member **120** contacts eye **130**. A vacuum is applied through vacuum port **210** to remove substantially all air trapped between eye-contact member **120** and eye **130**, such that contact device **110** is sealingly engaged with eye **130**. FIG. 7B illustrates the positioned and stabilized eye **130**. FIG. 7C shows downward, or Y-directional movement of control arm **180** of contact device **110**. In a preferred embodiment, movement of control arm **180** is performed by a trained medical professional. Upon directional displacement (e.g. X-Y control of arm **180**), control arm **180** pivots about spherical pivot **220** such that eye **130** is controllably moved and/or positioned. In one embodiment of the invention, sensor feedback provides the location of the eye **130**. In another embodiment, control arm **180** is connected to a drive mechanism, as illustrated in FIGS. 6A-6C, which allows automated control and position information of the eye **130** as it is moved or positioned.

With continuing reference to FIGS. 7A-7C, an exemplary method of utilizing the system of the invention includes rotating the eye prior to application of treatment. The eye can be gripped and rotated an amount, such as, for example about 1 to 2 degrees, or more broadly about 1 to 90 degrees, about the center point. In other implementations, the rotation may range from about 1 to about 45 degrees or more, and/or at different points in time, in different directions and/or in different amounts. Following such rotation, the eye may, or may not, be held in the rotated position, for example while some or all of the treatment(s) are applied. After application of some or all of the desired treatment, the eye can be moved back, to a full or partial extent, to its naturally-occurring orientation and/or can be released such that the eye moves, to a full or partial extent, back to its naturally-occurring orientation without assistance from the system.

In some embodiments of the invention, after application of some or all of the desired eye treatment(s), the eye can be rotated in the opposite direction to a greater extent than that to which it was first rotated, such as rotation in the counterclockwise direction about 1 to 90 degrees. Following any of the rotations of the eye described herein, and/or at any intermediate step, part or all of the eye being rotated and/or treated may be held (temporarily or permanently) by means in addition to the contact device **110** illustrated in FIGS. 7A-7C.

In other embodiments of the invention, following an initial stabilization and rotation, or positioning, of the eye, and application of one or more treatments to the eye (e.g., radiotherapy), the eye can be rotated in the same direction to a greater extent than to which it was first rotated. Then, one or more desired eye treatments can again be administered. The process can be repeated to form additional eye treatments to, for example, focus energy on a single spot, e.g., the macula, such that the sclera is minimally impacted. The eye can be rotated in the opposite direction (e.g., past the original, naturally occurring orientation) to various degrees to facilitate administration of one or more tissue treatments. Accordingly, the eye can be rotated in both directions to facilitate admin-

istration of treatment such that potential scleral damage and/or healing time can be attenuated or eliminated.

In one embodiment of the invention, the system includes a fluid dispenser. Fluids, including water, sterile water or conditioned fluids, such as those described in U.S. Pat. Nos. 5,785,521 and 6,350,123, the contents of which are incorporated herein by reference, may be added to assist with healing times or otherwise aid the treated tissue. For example, fluid may be applied by way of a small air mister, e.g., from a local or remotely disposed reservoir or dropper, affixed to the system. The fluid may be applied between and/or during application of treatment, to attenuate or eliminate charring and/or wash away blood. Alternatively, fluid may be applied using a sprayer line affixed to the treatment device, contact device or otherwise affixed on the system. The sprayer line may include tubing, e.g., clip-on and/or silicone based tubing, built into the system and a fluid dispensing unit. The fluid-dispensing input may be activated manually or automatically to power dispensation of fluid.

FIGS. 7A-7C also illustrate the application of a biasing force **155** by arm **180** during an eye-positioning procedure. As noted above, this force is used to hold the eye-contact member on the eye, such that the negative pressure between the eye and eye-contact member can function to stabilize the position of the eye, but at a relatively low vacuum. In this embodiment of the invention, an eye-contact assembly, indicated at **117**, includes an eye-contact member **120** and a biasing mechanism for biasing the eye-contact member against the patient's eye with a force of between 1-25 grams. In the embodiment illustrated, the biasing mechanism is contained within arm **120**, and indicated by direction-of-force arrow **119**. As noted above, the biasing mechanism may take the form of a coiled spring or circuit-activated solenoid that biases the arm in the direction of arrow **119**.

In another embodiment of the system, the eye-contact member may be supported on a track for sliding movement toward and away from the eye, along an axis substantially normal to the axis of the eye, where the track may be mounted, for example, on the head support for positioning in up-and-down and left-and-right directions, to place the track immediately in front of the patient's eye. With this positioning the eye-contact member can then be moved to engage the front of the patient's eye, with the patient looking straight ahead. Once initial contact is made, and after removing air from the eye/contact member interface, a biasing force can be applied to the contact member to hold to against the eye during a subsequent eye therapy procedure.

FIGS. 8A and 8B depict a mechanism by which the contact device **110** can be used to align the eye with laser alignment system **800**. Optionally, the alignment mechanism also directly aligns a treatment system, such as a radiotherapy system (not shown) in which the radiotherapy system directs its energy toward the eye in relation to the alignment system. Laser pointer beam **810** (which is collinear with the therapeutic beam in some embodiments) is emitted from laser system **800** through a collimator opening **820** and reflects off the surface of mirror **230** of the contact device **110**. In the non-alignment case depicted in FIG. 8A, the laser pointer beam **810** will not reflect off the surface of mirror **230** collinearly with the collimator opening **820**, but will be off-axis, as shown by reflection beam **830**. The orientation of the laser system **800** and/or the contact device **600** can be manually or automatically adjusted by direct visualization of the location of the reflection beam **830** or by sensors that detect the location of the reflection beam **830** and adjust the laser system **800** to bring the laser reflection beam **830** into alignment. In the case where the laser pointer is in fact aligned (FIG. 8B), the

laser pointer beam **810** is reflected, and the laser reflection beam **830** is substantially collinear with the laser pointer beam **830**. The system includes, in some embodiments, a sensing module that senses a position of the eye and relays information concerning the position of the eye to the position guide. The sensing module can include a portion that physically contacts the eye, which can include the eye-contact member **120** positionable on or over the cornea of the eye. The sensing module can, in some embodiments, optically sense the position of the eye with, for example, a laser.

Some embodiments of the invention, as shown in FIGS. **9-24**, provide that the eye-contact member have one or more apertures or portions of radiotranslucent material positioned radially around a center of the eye-contact member **120**. The apertures can be shaped as circles, squares, rectangles, ovals, curvilinear, irregular, annular, concentric rings, and so forth. In some embodiments, the contact device **110** is configured to include an aperture or portion of radiotranslucent material only in a center portion of the device to permit transmission of radiation therethrough to target tissue.

FIGS. **9-24** illustrate a variety of embodiments of eye-contact members that can be used to selectively control the therapeutic energy (e.g., radiotherapy) emitted through the eye-contact members toward the eye. FIG. **9** shows one embodiment of the eye-contact member **900**. As seen, the eye-contact member **900** includes a connector **905** for coupling the eye-contact member **900** to a control arm (not shown) as discussed above. The eye-contact member **900** is positioned onto an exterior surface of the eye. There is no aperture or opening located on the eye-contact member **900** as shown in FIG. **9**. FIG. **10** illustrates a circular aperture **1010** located off center of eye-contact member **1000**, which can be coupled to a control arm through connector **1005**. The circular aperture is preferably transmissive of energy to the eye of a subject when used in combination with a therapeutic treatment device, such as a radiotherapy device allowing precise control of energy through the eye onto a predetermined structure located within the eye, e.g., the macula. The diameter of the apertures can be of any range suitable for the treatment selected. In particular embodiments of the invention, the diameter of the aperture ranges from about 25 microns to about 200 microns. A 100 micron aperture is contemplated in one embodiment. In an alternative embodiment, a 200 micron diameter aperture is utilized.

FIGS. **11-18** are similar to the eye-contact member **1000**, except as set forth below. Accordingly, the eye-contact members described in connection with FIGS. **11-18** can be used and applied to the eye of a subject in a similar fashion to the eye-contact members **900** or **1000**. For example, FIG. **11** shows an embodiment of an eye-contact member **1100** that includes a connector **1105** and an aperture **1110** formed in the shape of a crescent. FIG. **12** shows another embodiment of an eye-contact member **1200** that includes a connector **1205** and an aperture **1210** formed in the shape of a heptagon. FIG. **13** shows another embodiment of an eye-contact member **1300** that includes a connector **1305** and a plurality of apertures **1310**, **1312**, **1314** formed in the shape of circles. FIG. **14** shows another embodiment of an eye-contact member **1400** that includes a connector **1405** and an aperture **1410** formed in the shape of a diamond. FIG. **15** shows another embodiment of an eye-contact member **1500** that includes a connector **1505** and an aperture **1510** formed in the shape of a partial circle located at the periphery of eye-contact member **1500**. FIG. **16** shows another embodiment of an eye-contact member **1600** that includes a connector **1605** and an aperture **1610** formed in the shape of a kidney. It will be appreciated that the apertures shown in FIGS. **11-12**, **14**, **16** and **18** are merely

exemplary of non-circular apertures. Other shapes and arrangements may also be provided and are within the scope of the present invention. FIG. **17** shows another embodiment of an eye-contact member **1700** that includes a connector **1705** and an aperture **1710** formed in the shape of a partial circle formed at the periphery of eye-contact member **1700**. FIG. **18** shows another embodiment of an eye-contact member **1800** that includes a connector **1805** and an overall shape that covers approximately half the area of an eye relative to the eye-contact member **900** of FIG. **9**. Thus, the eye-contact member **1800** may allow more treatment energy and/or easier access to the eye.

The eye-contact members of FIGS. **9-18** preferably have a constant thickness. However, in some embodiments, the thickness of the eye-contact members may vary between the outer periphery and the center of the eye-contact members. For example, the thickness of the eye-contact member may gradually decrease from the center to the periphery of the eye-contact member to allow more energy to enter the eye at the periphery than enters nearer the center. The eye-contact members are, in some embodiments at least partially and preferably completely opaque, outside the one or more aperture regions. The opacity of the eye-contact members may be achieved in any of several different ways. For example, in one embodiment, the material used to form the eye-contact member may be naturally opaque. Alternatively, the material used to form the eye-contact member may be substantially clear, but treated with a dye or other pigmentation agent to render a portion or all of the eye-contact member substantially or entirely opaque. In still another embodiment, one or both of the surfaces of the eye-contact members may be treated physically or chemically (such as by etching) to alter the refractive and transmissive properties of the eye-contact member making it less transmissive of energy.

In still another alternative, the surface of the eye-contact member may be treated with a particulate deposited thereon. For example, the surface of the eye-contact member may be deposited with particulate of titanium, gold or carbon to provide opacity to the surface of the eye-contact member. Radiopaque materials such as barium or florescent compounds can also be included. In another alternative, the particulate may be encapsulated within the interior of the eye-contact member. Finally, the eye-contact member may be patterned to provide areas of varying energy transmissivity, as generally shown in FIGS. **19-24**, which are discussed in detail below.

FIG. **19** shows an embodiment of an eye-contact member **1900** that includes a connector **1905** and a plurality of apertures **1910** in the pattern of radial spokes extending from the connector **1905** to an outer periphery of the eye-contact member **1900**. The apertures may have the same opacity, or alternatively have opacities that gradually increase or decrease, as desired. The graduated opacity may be achieved by, for example, providing different degrees of pigmentation to the apertures **1910**. In another embodiment, energy blocking materials of the type described above in variable degrees may be selectively deposited on the surface of the eye-contact member **1900**. FIG. **20** is a side view of the eye-contact member of FIG. **19** showing a plurality of radially extending slots **1910** emanating from the center **1905** of the eye-contact member.

In a similar manner, FIG. **21** shows an embodiment of an eye-contact member **2100** that includes a connector **2105** and a plurality of circular apertures **2110**, **2112** and **2114** that increase in diameter from the center to the periphery of eye-contact member **2100**. FIG. **22** is a side view of the eye-contact member of FIG. **21** showing a plurality of circular

shaped apertures **2110**, **2112**, **2214** increasing in size and radially spaced from the center **2205** of the eye-contact member **2200**.

FIG. **23** illustrates an embodiment of an eye-contact member **2305** which utilizes a patterned aperture structure which includes areas ranging that are opaque **2320** to areas that are transmissive of energy **2310**. FIG. **24** is a side view of the eye-contact member of FIG. **23** showing a grid of apertures **2310** within the eye-contact member **2300**.

In the embodiments described above, the selected treatment device is indirectly coupled to the contact device through attachments to the system. For example, in a preferred embodiment described above, the contact device is coupled to a control arm which is connected to the system through a drive mechanism; and the selected treatment device is coupled to the system such that the spatial relationship between the contact device and the selected treatment device can be dynamically determined. In an alternative embodiment of the present invention, there exists a direct physical connection between the contact device and the selected treatment system. Thus, in some embodiments, the physical connection can include a treatment coupling device. The coupling device has an eye-contact member which can include, for example, a scleral lens and a treatment device coupling surface. The eye-contact member can cover the cornea and contact the cornea or it can cover the cornea, only contacting the sclera. In some embodiments, the eye-contact member can cover and contact both the cornea and the sclera. The eye-contact member can be a lens in some embodiments, and in alternative embodiments, the eye-contact member can be a substantially transparent window with little or no refraction. The eye-contact member can be used to retain ocular gel or it can be shell with a hole in the center. The eye-contact member can be customized for an individual patient using imaging modalities, such as for example, an IOL master, optical coherence tomography (OCT), corneal surface mapping, MRI, CT scan, and ultrasound. The eye-contact member can be flexible or rigid or a composite. One or more flanges can function to hold the eyelids apart or can serve as a fiducial for the treatment device.

Opposite the eye-contact member are treatment device coupling surfaces, or portions. These surfaces, individually or collectively, couple the coupling device with the radiotherapy system. While the eye-contact member interfaces with the eye and structures, the treatment portion couples the eye-contact member to the treatment system. The treatment portion can link the coupling device to the treatment device in a variety of ways. For example, the treatment portion can couple to the treatment device via laser pointer, via infrared coupling, via microwave coupling, via mechanical coupling, via reflection, or via radiofrequency transmitters.

### III. Methods of the Invention

The device of the present invention may be used in a wide variety of ocular treatment methods. Preferred treatment methods include laser therapy and radiation therapy. As illustrated in FIG. **25**, a preferred method **2500** of employing the system described above includes preparing a subject's eye for treatment **2510** which can include delivering an anesthetic, taping the upper or lower lid, dilating the eye, measuring biometric parameters such as axial length, corneal diameter, etc. Following preparation, the subject's head is secured to the system **2520**. The contact device is then positioned on the subject's eye as referenced by reference numeral **2530**. Positioning of the holder (described above) on the eye is accomplished by aligning the center of the holder, using the x,y,z

movement, with the center of the limbus. This can be performed as an approximation by a physician while observing the both the holder and the eye of the patient directly or on a computer monitor. Alternatively, an imaging camera can determine the center of the limbus automatically and aid in the positioning of the holder with its center aligned with the center of the limbus. In some embodiments, the holder is positioned in place automatically rather than manually by the device operator.

Once the position of the holder relative to the limbus is determined, suction is applied through the holder to appose it to the eye **2532**. With the holder firmly attached to the eye, the holder (and eye) can be moved into position relative to the treatment device in known coordinates within the system. In the embodiment where the holder contains a mirror to monitor its reflection, the holder is positioned such that a reflection from the mirror is in position. Once the eye is in position, its movement is stabilized **2540** with suction in one example. The eye can then be positioned to a predetermined location relative to the treatment device, as indicated by numeral **2550**. The treatment device is then moved about, or otherwise positioned relative to, the eye to deliver its treatment **2560**. Alternatively, the treatment device moves into position about the eye. Method steps **2550-2560** can be repeated until a desired treatment is completed, after which the subject's eye is released from the contact device **2570**.

As described above and indicated by numeral **2534**, a quick release is built into the contact device in some embodiments of the invention. In case of an emergency or fatigue, the patient can release from the holder by applying a modicum of force which results in the eye-contact member breaking away from the remainder of the contact device. In such a case, the method step returns to the step prior to positioning and securing the head **2520**, or to the step of positioning the contact device on the subject's eye **2530**, as indicated in FIG. **25**.

An exemplary method for utilizing the system is now described. The method includes preparing the eye for positioning. Such preparation includes applying eye numbing drops to the eye of the subject. Scleral clearance can be provided by securing the lower eyelid downward with tape or eyelid eversion. The untreated eye is covered with a patch. The subject's head is positioned in a head support and the chin is rested on a chinrest. The head may be secured to the head support with straps or the like. The eye-contact member is placed on the cornea by tilting the eye-contact member to contact the upper portion of the sclera. As the eye-contact member contacts the upper scleral region of the eye, the eye-contact member is tilted downward to achieve full contact with the eye. Suction is then applied, and verified visually and by the vacuum source which "holds" suction. The contact device is then aligned with a laser, and centered on the limbus. A desired treatment procedure is then performed.

In a preferred embodiment of the method of the invention as illustrated in FIG. **26**, a method **2600** of treating an ocular structure of an eye with a radiation beam from a radiotherapy system is described, including contacting a surface of the eye with an eye-contact member, wherein the eye-contact member comprises a first portion, such that an axis passing through the ocular structure also passes through the first portion of the eye-contact member; and emitting a plurality of radiation beams toward the ocular structure **2610**, from a radiotherapy system located outside the eye, such that the plurality of radiation beams each have a trajectory that intersects the axis at a treatment site at the ocular structure, the treatment site being effectively treatable by at least one of the plurality of radiation beams. In the embodiment illustrated in FIG. **2600**,

at least a portion of the radiation is transmitted through the contact device which has been positioned on the eye. In an alternative embodiment, at least a portion of the radiation is transmitted to the eye without contacting any portion of the contact device. In yet another embodiment, which can be used as an alternative or in combination with the embodiments described above, at least a portion of the radiation is reflected off the contact device when the contact device is positioned on the eye **2630**. The radiation treatment is continued until a desired effect is achieved **2640**.

In another embodiment of a method of the invention **2700**, as illustrated in FIG. **27**, the cornea is reshaped using the system of the invention described above. In this embodiment, a laser is emitted toward the cornea of an eye **2710**, followed by the desired reshaping of the surface of the cornea **2720**. According to some embodiments of the invention, applying treatment energy (e.g., radiotherapy or ablating optical energy) to tissues (e.g., the conjunctiva or sclera) can refer to tissue treatment groupings and/or tissue treatment markings corresponding to tissue treatment groupings. Treatment can refer to two or more tissue treatments arranged in a focused spot or spots on the tissue; a nonlinear and nonarcuate grouping (e.g., pattern) on the tissue; and/or arranged in a plurality of focused spots, nonlinear and nonarcuate groupings on the tissue. Tissue treatments or groupings of tissue treatments may include focused spots, random line shapes, (straight, curved, or otherwise), or may include line shapes formed in a pattern that is predetermined based on a treatment customized to a tissue area.

In another embodiment, the system described above is used to stabilize an eye during laser photocoagulation of the retina or during a photodynamic treatment of the retina. In these treatments, stabilization of the eye is currently performed by the physician who holds the eye manually with a lens contacting the eye. A limitation of this technique is that the physician can only hold the lens with very limited positioning and stabilization ability subject to tremor and shake. Given the system above, the physician would be able to apply these treatments with confirmation of stability through the system camera stabilizing arm.

Particular implementations of lasers for use on, for example, the sclera may include Er:YAG, Er:YSGG, Er, CTE:YAG, or Cr:YSGG lasers operated at exemplary wavelengths ranging from about 2.7 to 2.9 microns; XeCl excimer lasers operated at an exemplary wavelength of about 308 nm; frequency-shifted solid state lasers operated at exemplary wavelengths of about 0.15 microns to about 3.2 microns; excimer lasers of ArF operated at a wavelength of about 93 nm; harmonic generations of Nd:YAG or Nd:YAL or Ti:sapphire lasers operated at wavelengths of about 190 nm to about 220 nm; CO lasers operated at a wavelength of, for example, about 6 microns and carbon dioxide lasers operated at a wavelength of, for example, about 10.6 microns; diode lasers operated at exemplary wavelengths of about 0.8 microns to about 2.1 microns; gas lasers operated at wavelengths of about 2.6 microns to about 3.2 microns; and other gas or solid state lasers including flash-lamp and diode-laser pumped lasers operated at wavelengths of about 0.5 microns to about 10.6 microns; and optical parametric oscillation (OPO) lasers operated at exemplary wavelengths of about 2.6 microns to about 3.2 microns.

Thus, the devices and methods described above are useful, in some embodiments of the invention, to treat conditions of the eye of a subject. Sources of treatment energy, such as electromagnetic energy emitting devices, can be utilized to implement corneal and/or non-corneal manipulations. According to the architectures and techniques of some

embodiments of the invention, the source or sources (when utilized in combination) can be activated to direct energy onto and/or into parts of the eye, such as the conjunctiva and sclera to treat conditions such as presbyopia, wherein the energy affects at least one property of the eye and results in an enhancement in a property of the eye.

In some embodiments of the invention, focusing disorders such as myopia and hyperopia are treated. Myopia, or nearsightedness, relates to an eyesight refractive abnormality whereby distant objects appear blurred as a result of rays of light entering the eye being brought to focus in front of the retina. Hyperopia, or farsightedness, on the other hand, relates to an eyesight refractive abnormality whereby near objects appear blurred or fuzzy as a result of light rays being brought to focus behind the retina.

One variation of hyperopia is presbyopia, which typically is associated with a person's lack of capacity to focus at near distances and which tends to develop and progress with age. Regarding this progression, presbyopia is thought to advance as the eye progressively loses its ability to accommodate or focus sharply for near vision with increasing age of the person. Accordingly, the condition of presbyopia generally signifies a universal decrease in the amplitude of accommodation of the affected person.

Myopia and hyperopia can be treated surgically using techniques including corneal interventions, such as reshaping a surface curvature of the cornea located inside of the limbus area, and non-corneal manipulations, such as altering properties of the sclera (which is located outside of the limbus area), ciliary muscle, zonules, or lens. An example of the former treatment includes ablating the surface of the cornea itself to form a multifocal arrangement (e.g., distance vision in one eye and reading vision in another eye according to a treatment plan referred to as monovision) facilitating viewing by a patient of both near and far objects. An example of the latter treatment includes introducing kerfs into portions of the sclera to thereby increase accommodation. Non-corneal interventions typically include temporarily removing or pulling back the subject's conjunctiva, using forceps and scissors and/or one or more of scalpels, cautery, plasma, and laser methods, followed by the actual non-corneal manipulations (e.g., forming kerfs in the sclera). After completing the kerfs, the conjunctiva is then typically sutured back into position.

Electromagnetic energy devices may include, for example, lasers emitting a wide range of wavelengths, such as lasers having wavelengths ranging, for example, from about 0.2 microns to about 3.1 microns. Exemplary laser beam sizes can range from about 0.005 mm up to about 1.0 mm, or 2.0 mm. Exemplary laser energy per pulse values can range from about 0.1 mJ to about 50 mJ depending on, for example, the pulse duration and the laser beam spot size. Typical pulse laser widths may range from about 150 nanoseconds to about 1000 microseconds. The areas to be treated can be pre-traced with a vascular laser or long pulse Er, Cr:YSGG, or long pulse Er:YAG, to minimize bleeding.

In one embodiment of the invention, radiotherapy is administered. Radiotherapy is particularly useful for treating macular degeneration. Macular degeneration is a condition where the light-sensing cells of the macula, a near-center portion of the retina of the human eye, malfunction and slowly cease to work. Macular degeneration is the leading cause of central vision loss in people over the age of fifty years. Clinical and histologic evidence indicates that macular degeneration is in part caused by or results in an inflammatory process that ultimately causes destruction of the retina. The inflammatory process can result in direct destruction of the retina or destruction via formation of neovascular membranes

which leak fluid and blood into the retina, quickly leading to scarring. In treating macular degeneration, the patient's macula is identified as the target region of interest. After stabilizing and positioning the eye, in accordance with the methods described above, a source of soft collimated x-rays beams is moved to a position to direct the beam at the macular region of the eye, along a path through an outer side region of the eye that makes an angle with an axis normal to the cornea of the eye between 5-45 degrees, and preferably at an angle that avoids directing the beam through the lens of the eye. In one preferred treatment method, the beam source is moved, at the same angle with respect to normal, to tilted positions in which the beam is aimed at the macula from a slightly elevated position, and from a corresponding below-elevation condition, such that the macula is irradiated along different paths, to minimize the radiation seen by the eye along any one path.

Radiotherapy can be used in combination with other therapeutics for the eye. Radiotherapy can be used to limit the side effects of other treatments or can work synergistically with other therapies. For example, radiotherapy can be applied to laser burns on the retina or to implants or surgery on the anterior region of the eye. Radiotherapy can be combined with one or more pharmaceutical, medical treatments, and/or photodynamic treatments or agents. For example, radiotherapy can be used in conjunction with anti-VEGF treatment, VEGF receptors, steroids, anti-inflammatory compounds, DNA binding molecules, oxygen radical forming therapies, oxygen carrying molecules, porphyrin molecules/therapies, gadolinium, particulate based formulations, oncologic chemotherapies, heat therapies, ultrasound therapies, and laser therapies.

In some embodiments, radiosensitizers and/or radioprotectors can be combined with treatment to decrease or increase the effects of radiotherapy, as discussed in Thomas, et al., Radiation Modifiers: Treatment Overview and Future Investigations, *Hematol. Oncol. Clin. N. Am.* 20 (2006) 119-139; Senan, et al., Design of Clinical Trials of Radiation Combined with Antiangiogenic Therapy, *Oncologist* 12 (2007) 465-477; the entirety of both of these articles are incorporated by reference herein. Some embodiments include radiotherapy with the following radiosensitizers and/or treatments: 5-fluorouracil, fluorinated pyrimidine antimetabolite, anti-S phase cytotoxin, 5-fluorouridine triphosphate, 2-deoxyfluorouridine monophosphate (Fd-UMP), and 2-deoxyfluorouridine triphosphate capecitabine, platinum analogues such as cisplatin and carboplatin, fluoropyrimidine, gemcitabine, antimetabolites, taxanes, docetaxel, topoisomerase I inhibitors, Irinotecan, cyclo-oxygenase-2 inhibitors, hypoxic cell radiosensitizers, antiangiogenic therapy, bevacizumab, recombinant monoclonal antibody, ras mediation and epidermal growth factor receptor, tumor necrosis factor vector, adenoviral vector Egr-RNF (Ad5.Egr-TNF), and hyperthermia. In some embodiments, embodiments include radiotherapy with the following radioprotectors and/or treatments: amifostine, sucralfate, cytoprotective thiol, vitamins and antioxidants, vitamin C, tocopherol-monoglucoside, pentoxifylline, alpha-tocopherol, beta-carotene, and pilocarpine.

Antiangiogenic Agents (AAs) aim to inhibit growth of new blood vessels. Bevacizumab is a humanized monoclonal antibody that acts by binding and neutralizing VEGF, which is a ligand with a central role in signaling pathways controlling blood vessel development. Findings suggest that anti-VEGF therapy has a direct antivasular effect in human tissues. In contrast, small molecule tyrosine kinase inhibitors (TKIs) prevent activation of VEGFRs, thus inhibiting downstream signaling pathways rather than binding to VEGF directly.

Vascular damaging agents (VDAs) cause a rapid shutdown of established vasculature, leading to secondary tissue death. The microtubule-destabilizing agents, including combretastatins and ZD6126, and drugs related to 5,6-dimethylxanthine-4-acetic acid (DMXAA) are two main groups of VDAs. Mixed inhibitors, including agents such as EGFR inhibitors or neutralizing agents and cytotoxic anticancer agents can also be used.

Thus, the system of the present invention can be used in some embodiments to provide radiotherapy treatment. A treatment axis which provides a reference about which application of the radiation beams are applied can be coupled to or aligned with a system axis of the radiotherapy system, about which an x-ray source can be rotated. The x-ray source can rotate about the system axis of the radiotherapy device, about which the x-ray source can be rotated. The x-ray source can rotate about the system axis with or independent from an imaging subsystem and its corresponding axis. With the treatment axis aligned with the system axis, and with the coupling device engaging the eye, trajectories of the radiation beams can be determined to direct the radiation beams to be coincident with the target tissue of the eye of the subject. The defined space of the treatment axis, the system axis, the location of the coupling device, and the location of the x-ray source provides a confined coordinate frame that can be used, for example, for directing orientation and administration of the radiation beams.

In one embodiment of the invention, radiodynamic therapy is administered. Radiodynamic agents can be administered either systemically or into the vitreous; the region in the eye to be treated is then directly targeted with radiotherapy as described above. The targeted region can be precisely localized using the device of the invention and/or in combination with an eye model, and then radiation can be precisely applied to that region. Beam sizes of about 1 mm or less can be used in radiodynamic therapy to treat ocular disorders if the target is drusen for example. In other examples, the beam size is less than about 6 mm.

It is further contemplated that the system of the present invention can be utilized to treat a variety of types of cancer of the eye. Exemplary cancer treatments are described below.

Intraocular melanoma starts from pigment cells called melanocytes, which are found in the part of the eye known as the uvea. The uvea includes the iris, which forms the colored part of the eye; the ciliary body, which helps change the shape of the lens inside the eye so that it can focus; and the choroid, which is a very deep layer of the eye. Though it is uncommon, uveal melanoma is the most common primary eye tumor in adults; approximately 1200 people are diagnosed with the disease each year in the United States. Factors associated with the disease's development include light skin color, environmental exposure and genetic predisposition.

If the melanoma begins in the iris, it may appear as a dark spot on the eye. However, if it begins in the ciliary body or choroid, symptoms may appear as vision problems, if at all. In these cases, the disease is usually detected during a routine examination. Chances of recovery and response to treatment depend on the location of the melanoma and whether it has spread. Posterior uveal tract melanomas (those cancers arising from the ciliary body or the choroid—the deeper parts of the eye) are typically more malignant, with a five-year mortality rate of 30% when the tumor has spread to areas outside of the eye. Anterior uveal tract melanomas (those arising from the iris) have a 2% to 3% mortality rate over five years. Thus, in one embodiment of the invention, intraocular melanoma is treated using the system of the invention.

Standard treatment for intraocular melanoma typically includes surgical removal of the eye, or enucleation. Because of this procedure's effect on a patient's appearance, possible diagnostic uncertainties and the potential for the cancer to spread, alternative treatments have been introduced. These treatments include radiation with radioactive plaques, laser photocoagulation, transpupillary thermotherapy and cryotherapy. Also contemplated is proton beam therapy which has the ability to precisely target eye tumors without causing any serious damage to healthy tissue surrounding the eye.

Choroidal metastasis occurs when cancer spreads to the choroidal layer of the eye from another primary site, like the breast. In these situations, the goal of treatment is to improve the patient's quality of life by preserving vision and preventing removal of the eye. Chemotherapy, external beam radiation therapy and proton therapy in combination with the system described above are contemplated by the present invention for the treatment of choroidal metastasis such that the therapeutic treatment allows for retention of the eye, achieves a high probability of local control, and helps avoid vision loss and pain.

Retinoblastoma is an uncommon childhood cancer. It begins in the retina, and accounts for about 3% of cancers in children younger than 15 years—about 4 cases per million. It most often occurs before the age of two, with 95% of retinoblastoma diagnosed before the age of five. The tumor may affect one eye (about 75% of cases), or both eyes (25% of cases). More than 90% of retinoblastoma that does not spread beyond the eye will be cured. Retinoblastoma is sometimes caused by an inherited gene mutation; when it occurs in both eyes, it is always the result of a gene mutation. Treatment of retinoblastoma in accordance with the present invention contemplates a multidisciplinary approach, and involves treating the cancer as well as retaining vision. If the tumor is especially large, or if there is little expectation of retaining normal vision, surgery may be considered. Other options include cryotherapy, photocoagulation, chemotherapy and radiation therapy. External beam radiation therapy with protons has been used in select cases to control tumors. Proton therapy in combination with the system of the invention is also contemplated by the present invention.

Choroidal hemangiomas are benign vascular tumors that are usually well contained, and may cause a decrease in visual abilities. Treatment of choroidal hemangiomas is meant to reduce fluid collection under the retina and decrease the size of the tumor. Standard treatment involves laser photocoagulation, which successfully reattaches the retina, but may not always completely destroy the tumor. In recent years, radioactive plaque treatment and proton beam radiation treatments have been used. Proton beam therapy shares the precise tumor targeting ability of radioactive plaques, and is therefore contemplated for use with the system of the present invention.

In addition to the cancer treatment methods described above, the invention also contemplates manipulating the eye so as to move critical structures away from the treatment axis to deliver therapeutic amounts of radiation to tumors outside, but near, the eye. Thus, in one embodiment of the invention, the system is used to position the eye for the treatment of extraocular conditions.

In one embodiment of the invention, the device described above is utilized in combination with other therapeutics for the eye. For example, one or more therapy treatments such as cryotherapy, photocoagulation, chemotherapy and radiation therapy can be utilized in combination with the system of the present invention to provide therapeutic treatment of the eye.

From the foregoing, it can be seen how various objects and features of the invention are met. While certain aspects and

embodiments of the disclosure have been described, these have been presented by way of example only, and are not intended to limit the scope of the disclosure. The methods and systems described herein may be embodied in a variety of other forms without departing from the spirit thereof. All publications and patents cited herein are expressly incorporated herein by reference for the purpose of describing and disclosing systems and methodologies which might be used in connection with the invention.

It is claimed:

1. A system for performing an ocular irradiation procedure on a patient's eye, comprising

- (a) a head support for supporting the patient's head,
- (b) an eye-contact device attachable to the front portion of the patient's eye, to stabilize the position of the eye relative to the eye-contact device,
- (c) means for determining the position of the patient's eye, the eye being stabilized with respect to the contact device, and with the patient's head supported in the head support, in an external coordinate system,
- (d) a source of a collimated irradiation beam, and
- (e) a beam-positioning assembly for positioning the beam source in the external coordinate system such that the beam, when activated, is aimed along a selected path at a selected coordinate in the external coordinate system corresponding to a selected target region in the patient's eye;

wherein said determining means includes a position detector for determining the position of the contact device, and thus the position of the patient's eye attached to the contact device, in the external coordinate system;

wherein the system further includes an eye-positioning assembly for moving the eye-contact device to place the device at a selected position in the external coordinate system, and the position detector is operable to determine the position of the contact device in the external coordinate system, with such placed at said selected position;

wherein the eye-positioning assembly is operable to adjust the angular position of the contact device with respect to the patient's head, and the position detector detects an angle of a beam emanating from the contact device;

wherein the eye-contact device includes (i) a concave contact surface adapted to be placed against the front surface of a patient's eye, (ii) an outer surface, (iii) a port in fluid communication with the contact surface, by which a negative pressure can be applied between the eye and the contact surface, to stabilize the position of the eye with respect to the contact device, and (iv) a connector carried on the outer surface of the device, and the system further includes a biasing mechanism coupled to the connector of the contact device for pressing the eye-contact device against the eye with a force sufficient to hold the contact device against the eye, when the eye is stabilized with respect to the device by application of a negative pressure between the eye and the device's contact surface;

wherein the eye-positioning assembly includes an arm that is pivotally attached to the connector of the eye-contact device, and an arm control mechanism for controlling the movement of the arm in at least one direction in the external coordinate system, and the position detector is operable to determine the position of the contact device in the external coordinate system from the position of the eye-positioning assembly arm in the external coordinate system;

wherein said determining means includes a reference-beam light source operatively connected to the irradiation-beam source, for producing a reference light beam along a path coincident with the collimated irradiation beam produced by the irradiation beam source, and said beam-positioning assembly is operable to place the irradiation beam source at a position such that the collimated irradiation beam is aimed at the selected target region of patient's eye.

2. The system of claim 1, wherein the position detector includes a plurality of beam elements mounted on the contact device, for directing beams in accordance with the position and orientation of the beam elements, sensors for detecting the directions of the beams, and a processor for determining from the detected beam directions, the position and orientation of the contact device in the external coordinate system.

3. The system of claim 1, which further includes a vacuum source operable to apply a negative pressure of between about 20-50 mm Hg to the contact device contact surface.

4. The system of claim 1, for use in treating macular degeneration in a patient eye, wherein the beam source is a source of soft collimated x-rays, and the beam-positioning assembly is operable to position the beam source to direct a collimated x-ray beam at the macular region of the eye, along a path through an outer side region of the eye that makes an angle with an axis normal to the cornea of the eye, between about 5 and 45 degrees.

5. The system of claim 1, wherein the eye-contact device is a curved structure which is centered on a center axis extending through the contact device, substantially normal thereto, and said connector is disposed along the center axis of the contact device.

6. The system of claim 1, wherein the eye-contact device is a curved structure which is centered on a center axis extending through the contact device, substantially normal thereto, and said connector is disposed along an axis offset from the center axis.

7. The system of claim 1, wherein the connector is detachably coupled to the biasing mechanism, allowing the mechanism to break away from the eye-contact device when an above-threshold force is applied by or to the eye.

8. A system for performing an ocular irradiation procedure on a patient's eye, comprising

- (a) a head support for supporting the patient's head,
- (b) an eye-contact device attachable to the front portion of the patient's eye, to stabilize the position of the eye relative to the eye-contact device,
- (c) means for determining the position of the patient's eye, with the eye being stabilized with respect to the contact device, and with the patient's head supported in the head support, in an external coordinate system,
- (d) a source of a collimated irradiation beam, and
- (e) a beam-positioning assembly for positioning the beam source in the external coordinate system such that the beam, when activated, is aimed along a selected path at a selected coordinate in the external coordinate system corresponding to a selected target region in the patient's eye;
- (f) a position detector for determining the position of the contact device, and thus the position of the patient's eye attached to the contact device, in the external coordinate system
- (g) an eye-positioning assembly operable to adjust the angular position of the contact device with respect to the patient's head, the position detector being operable to detect an angle of a beam emanating from the contact device;

wherein the eye-contact device includes (i) a concave contact surface adapted to be placed against the front surface of a patient's eye, (ii) an outer surface, (iii) a port in fluid communication with the contact surface, by which a negative pressure can be applied between the eye and the contact surface, to stabilize the position of the eye with respect to the contact device, and (iv) a connector carried on the outer surface of the device, and the system further includes a biasing mechanism coupled to the connector of the contact device for pressing the eye-contact device against the eye with a force sufficient to hold the contact device against the eye, when the eye is stabilized with respect to the device by application of a negative pressure between the eye and the device's contact surface;

wherein the eye-positioning assembly includes an arm that is pivotally attached to the connector of the eye-contact device, and an arm control mechanism for controlling the movement of the arm in at least one direction in the external coordinate system, and the position detector is operable to determine the position of the contact device in the external coordinate system from the position of the eye-positioning assembly arm in the external coordinate system;

wherein said determining means includes a reference-beam light source operatively connected to the irradiation-beam source, for producing a reference light beam along a path coincident with the collimated irradiation beam produced by the irradiation beam source, and said beam-positioning assembly is operable to place the irradiation beam source at a position such that the collimated irradiation beam is aimed at the selected target region of patient's eye.

9. The system of claim 8, wherein the position detector includes a plurality of beam elements mounted on the contact device, for directing beams in accordance with the position and orientation of the beam elements, sensors for detecting the directions of the beams, and a processor for determining from the detected beam directions, the position and orientation of the contact device in the external coordinate system.

10. The system of claim 8, which further includes a vacuum source operable to apply a negative pressure of between about 20-50 mm Hg to the contact device contact surface.

11. The system of claim 8, for use in treating macular degeneration in a patient eye, wherein the beam source is a source of soft collimated x-rays, and the beam-positioning assembly is operable to position the beam source to direct a collimated x-ray beam at the macular region of the eye, along a path through an outer side region of the eye that makes an angle with an axis normal to the cornea of the eye, between about 5 and 45 degrees.

12. The system of claim 8, wherein the eye-contact device is a curved structure which is centered on a center axis extending through the contact device, substantially normal thereto, and said connector is disposed along the center axis of the contact device.

13. The system of claim 8, wherein the eye-contact device is a curved structure which is centered on a center axis extending through the contact device, substantially normal thereto, and said connector is disposed along an axis offset from the center axis.

14. The system of claim 8, wherein the connector is detachably coupled to the biasing mechanism, allowing the mechanism to break away from the eye-contact device when an above-threshold force is applied by or to the eye.