

US008693802B2

(12) **United States Patent**
Watanabe et al.

(10) **Patent No.:** **US 8,693,802 B2**
(45) **Date of Patent:** **Apr. 8, 2014**

(54) **FLUOROSCOPY APPARATUS,
FLUOROSCOPY SYSTEM, AND
FLUORESCENCE-IMAGE PROCESSING
METHOD**

(71) Applicant: **Olympus Corporation**, Tokyo (JP)

(72) Inventors: **Toshiaki Watanabe**, Tokyo (JP);
Yasushige Ishihara, Tokyo (JP)

(73) Assignee: **Olympus Corporation**, Tokyo (JP)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **13/834,395**

(22) Filed: **Mar. 15, 2013**

(65) **Prior Publication Data**
US 2013/0200273 A1 Aug. 8, 2013

Related U.S. Application Data

(60) Division of application No. 13/235,886, filed on Sep. 19, 2011, now Pat. No. 8,472,749, which is a continuation of application No. PCT/JP2010/054510, filed on Mar. 17, 2010.

(30) **Foreign Application Priority Data**
Mar. 24, 2009 (JP) 2009-072852

(51) **Int. Cl.**
G06K 9/00 (2006.01)

(52) **U.S. Cl.**
USPC **382/274**; 382/128; 382/162; 382/166

(58) **Field of Classification Search**
USPC 382/128-134, 162-167, 274
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

7,260,248	B2 *	8/2007	Kaufman et al.	382/128
8,031,938	B2 *	10/2011	Edge	382/167
2003/0144585	A1	7/2003	Kaufman et al.	
2004/0240716	A1 *	12/2004	de Josselin de Jong et al.	382/128

(Continued)

FOREIGN PATENT DOCUMENTS

JP	62-247232	10/1987
JP	2001-137173	5/2001
JP	2001-169999	A 6/2001
JP	2005-185452	A 7/2005
JP	2008-183349	A 8/2008

OTHER PUBLICATIONS

International Search Report dated May 11, 2010 issued in corresponding International Application No. PCT/JP2010/054510.

(Continued)


Primary Examiner — Wesley Tucker

(74) *Attorney, Agent, or Firm* — Scully, Scott, Murphy & Presser, P.C.

(57) **ABSTRACT**

A fluoroscopy apparatus including: an illumination unit having a light source radiating illumination light and excitation light onto an observation target, a fluorescence-imaging unit acquiring a fluorescence image by imaging fluorescence generated at the observation target by the excitation light, a white-light-imaging unit acquiring a reference image by imaging light returning from the observation target by the illumination light, and an image-correction unit obtaining a correction fluorescence image by raising the luminance value of the fluorescence image to the power of a reciprocal of a first and second exponent obtained by a power approximation of a distance characteristic of luminance versus observation distance, for the fluorescence image, and that obtains a corrected fluorescence image by dividing the correction fluorescence image by the correction reference image.

20 Claims, 26 Drawing Sheets

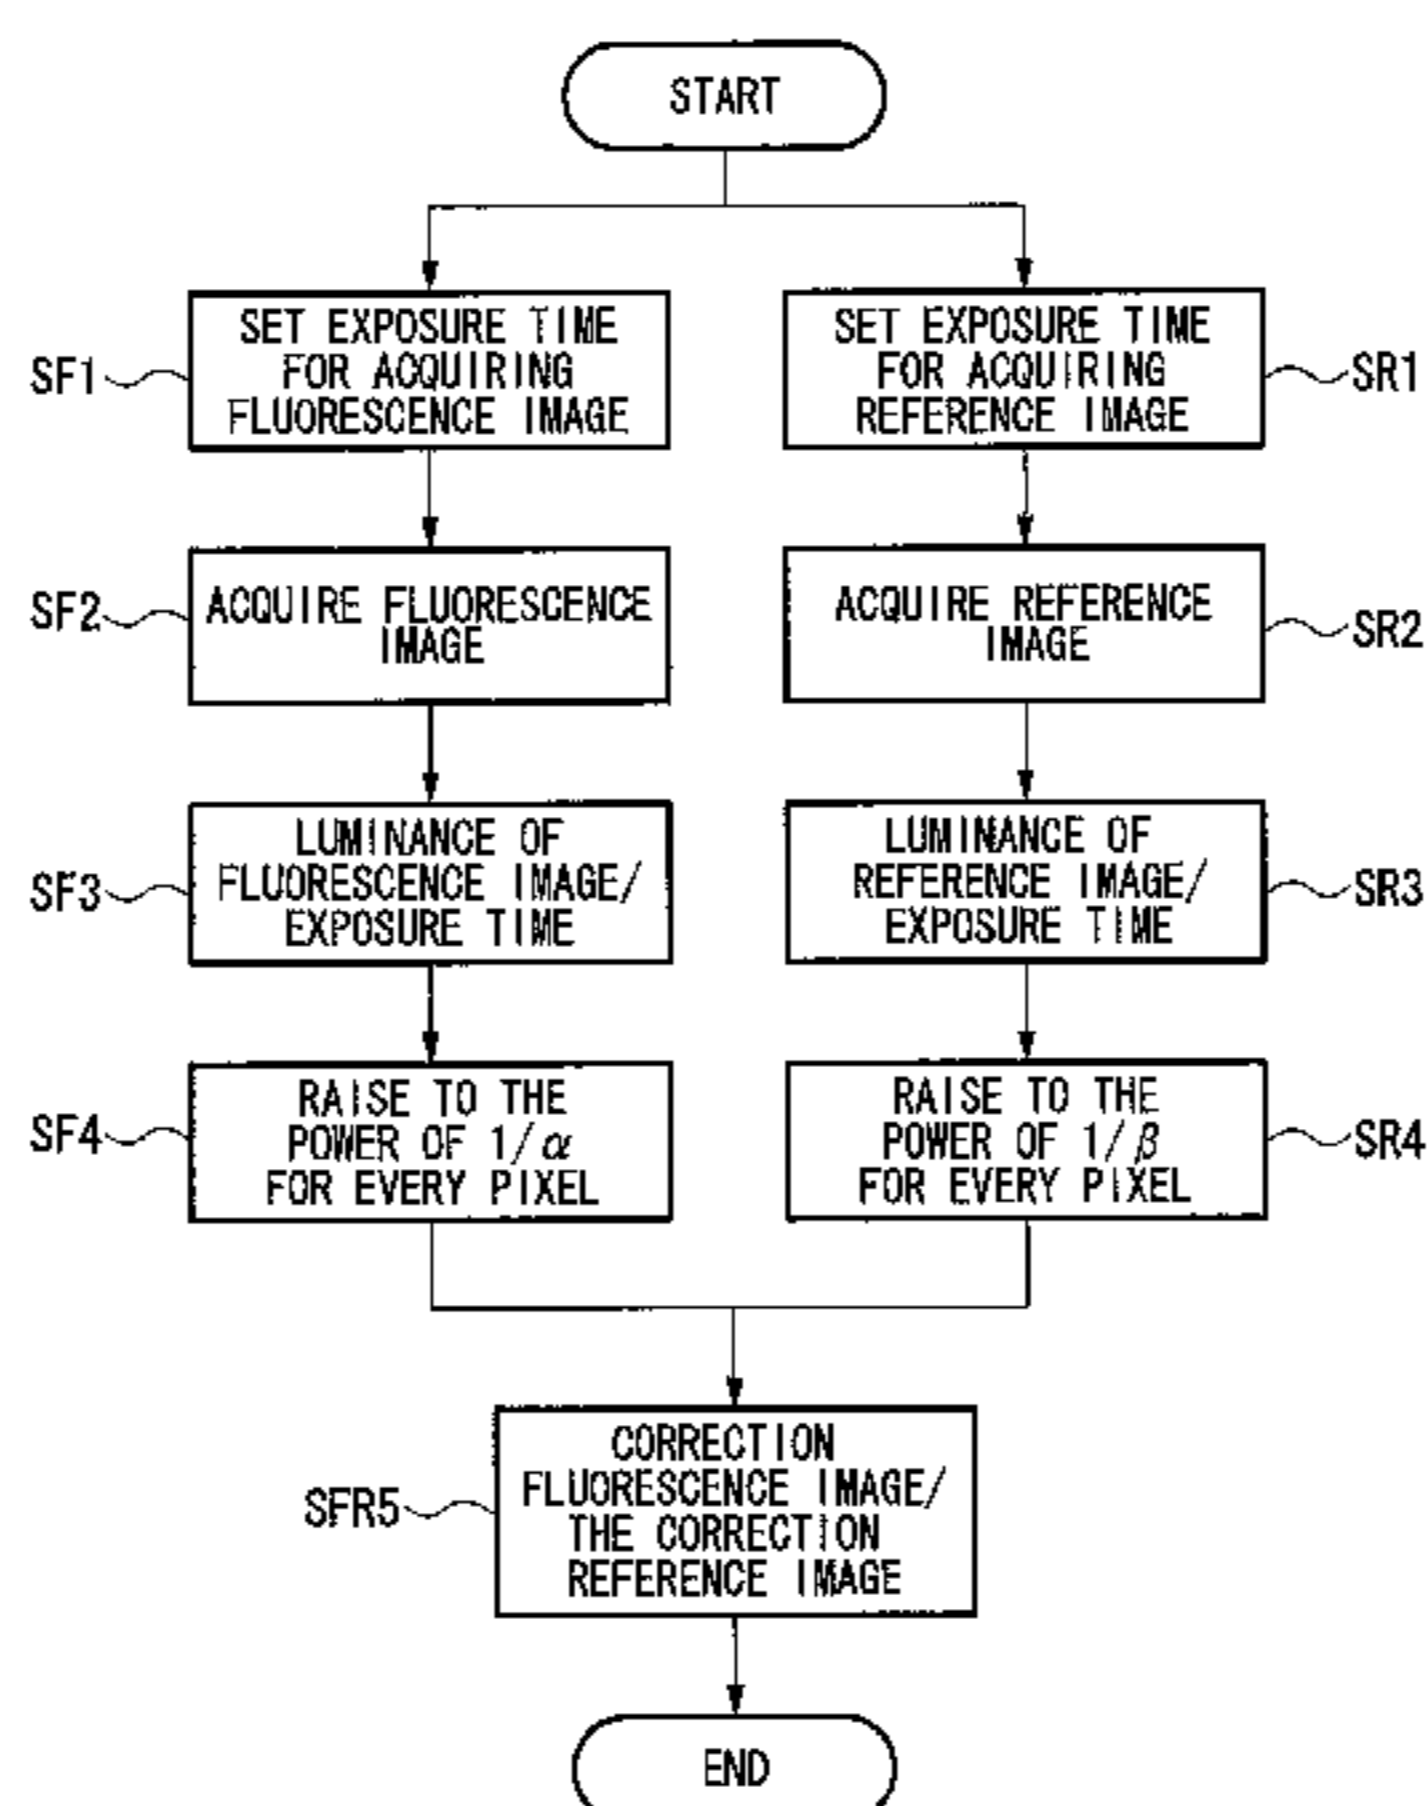

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0247624 A1* 10/2008 Scholz 382/131
2008/0255426 A1 10/2008 Iketani
2010/0292543 A1* 11/2010 Levitt et al. 600/300

2013/0028501 A1* 1/2013 Ishihara 382/132

OTHER PUBLICATIONS

Notice of Allowance and Issue Fee Due dated Feb. 28, 2013 issued in corresponding U.S. Appl. No. 13/235,886.

* cited by examiner

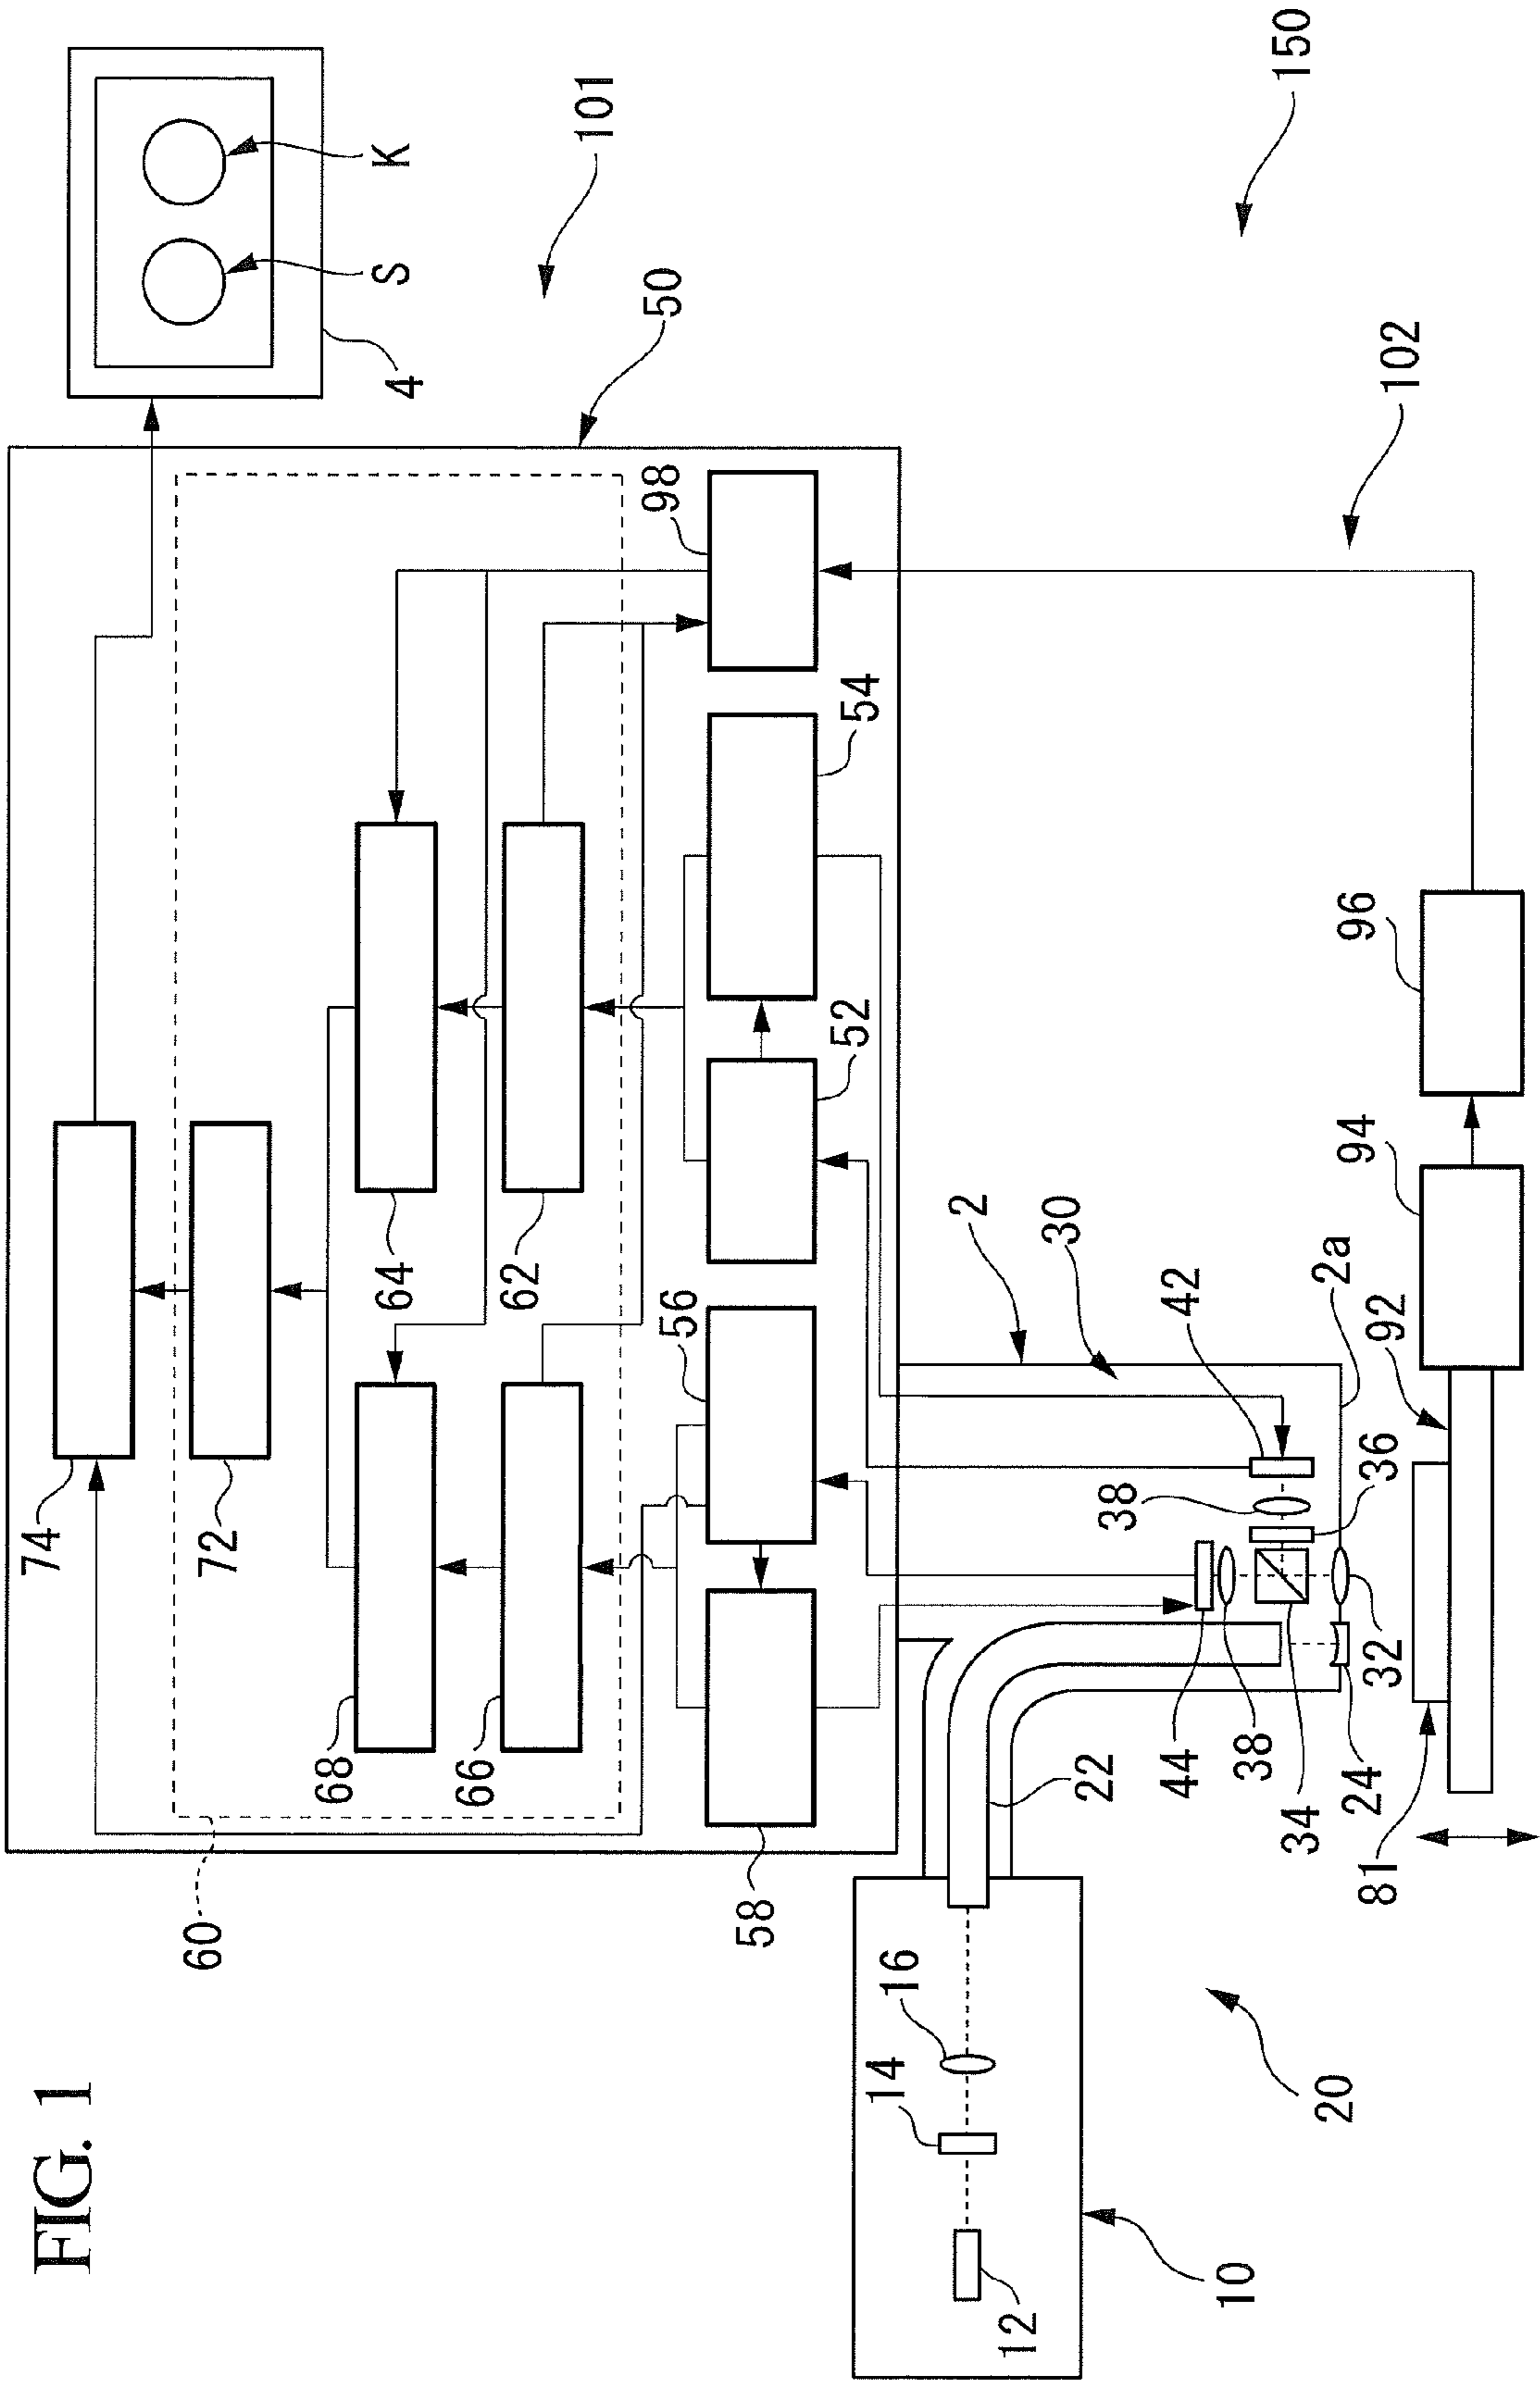


FIG. 1

FIG. 2

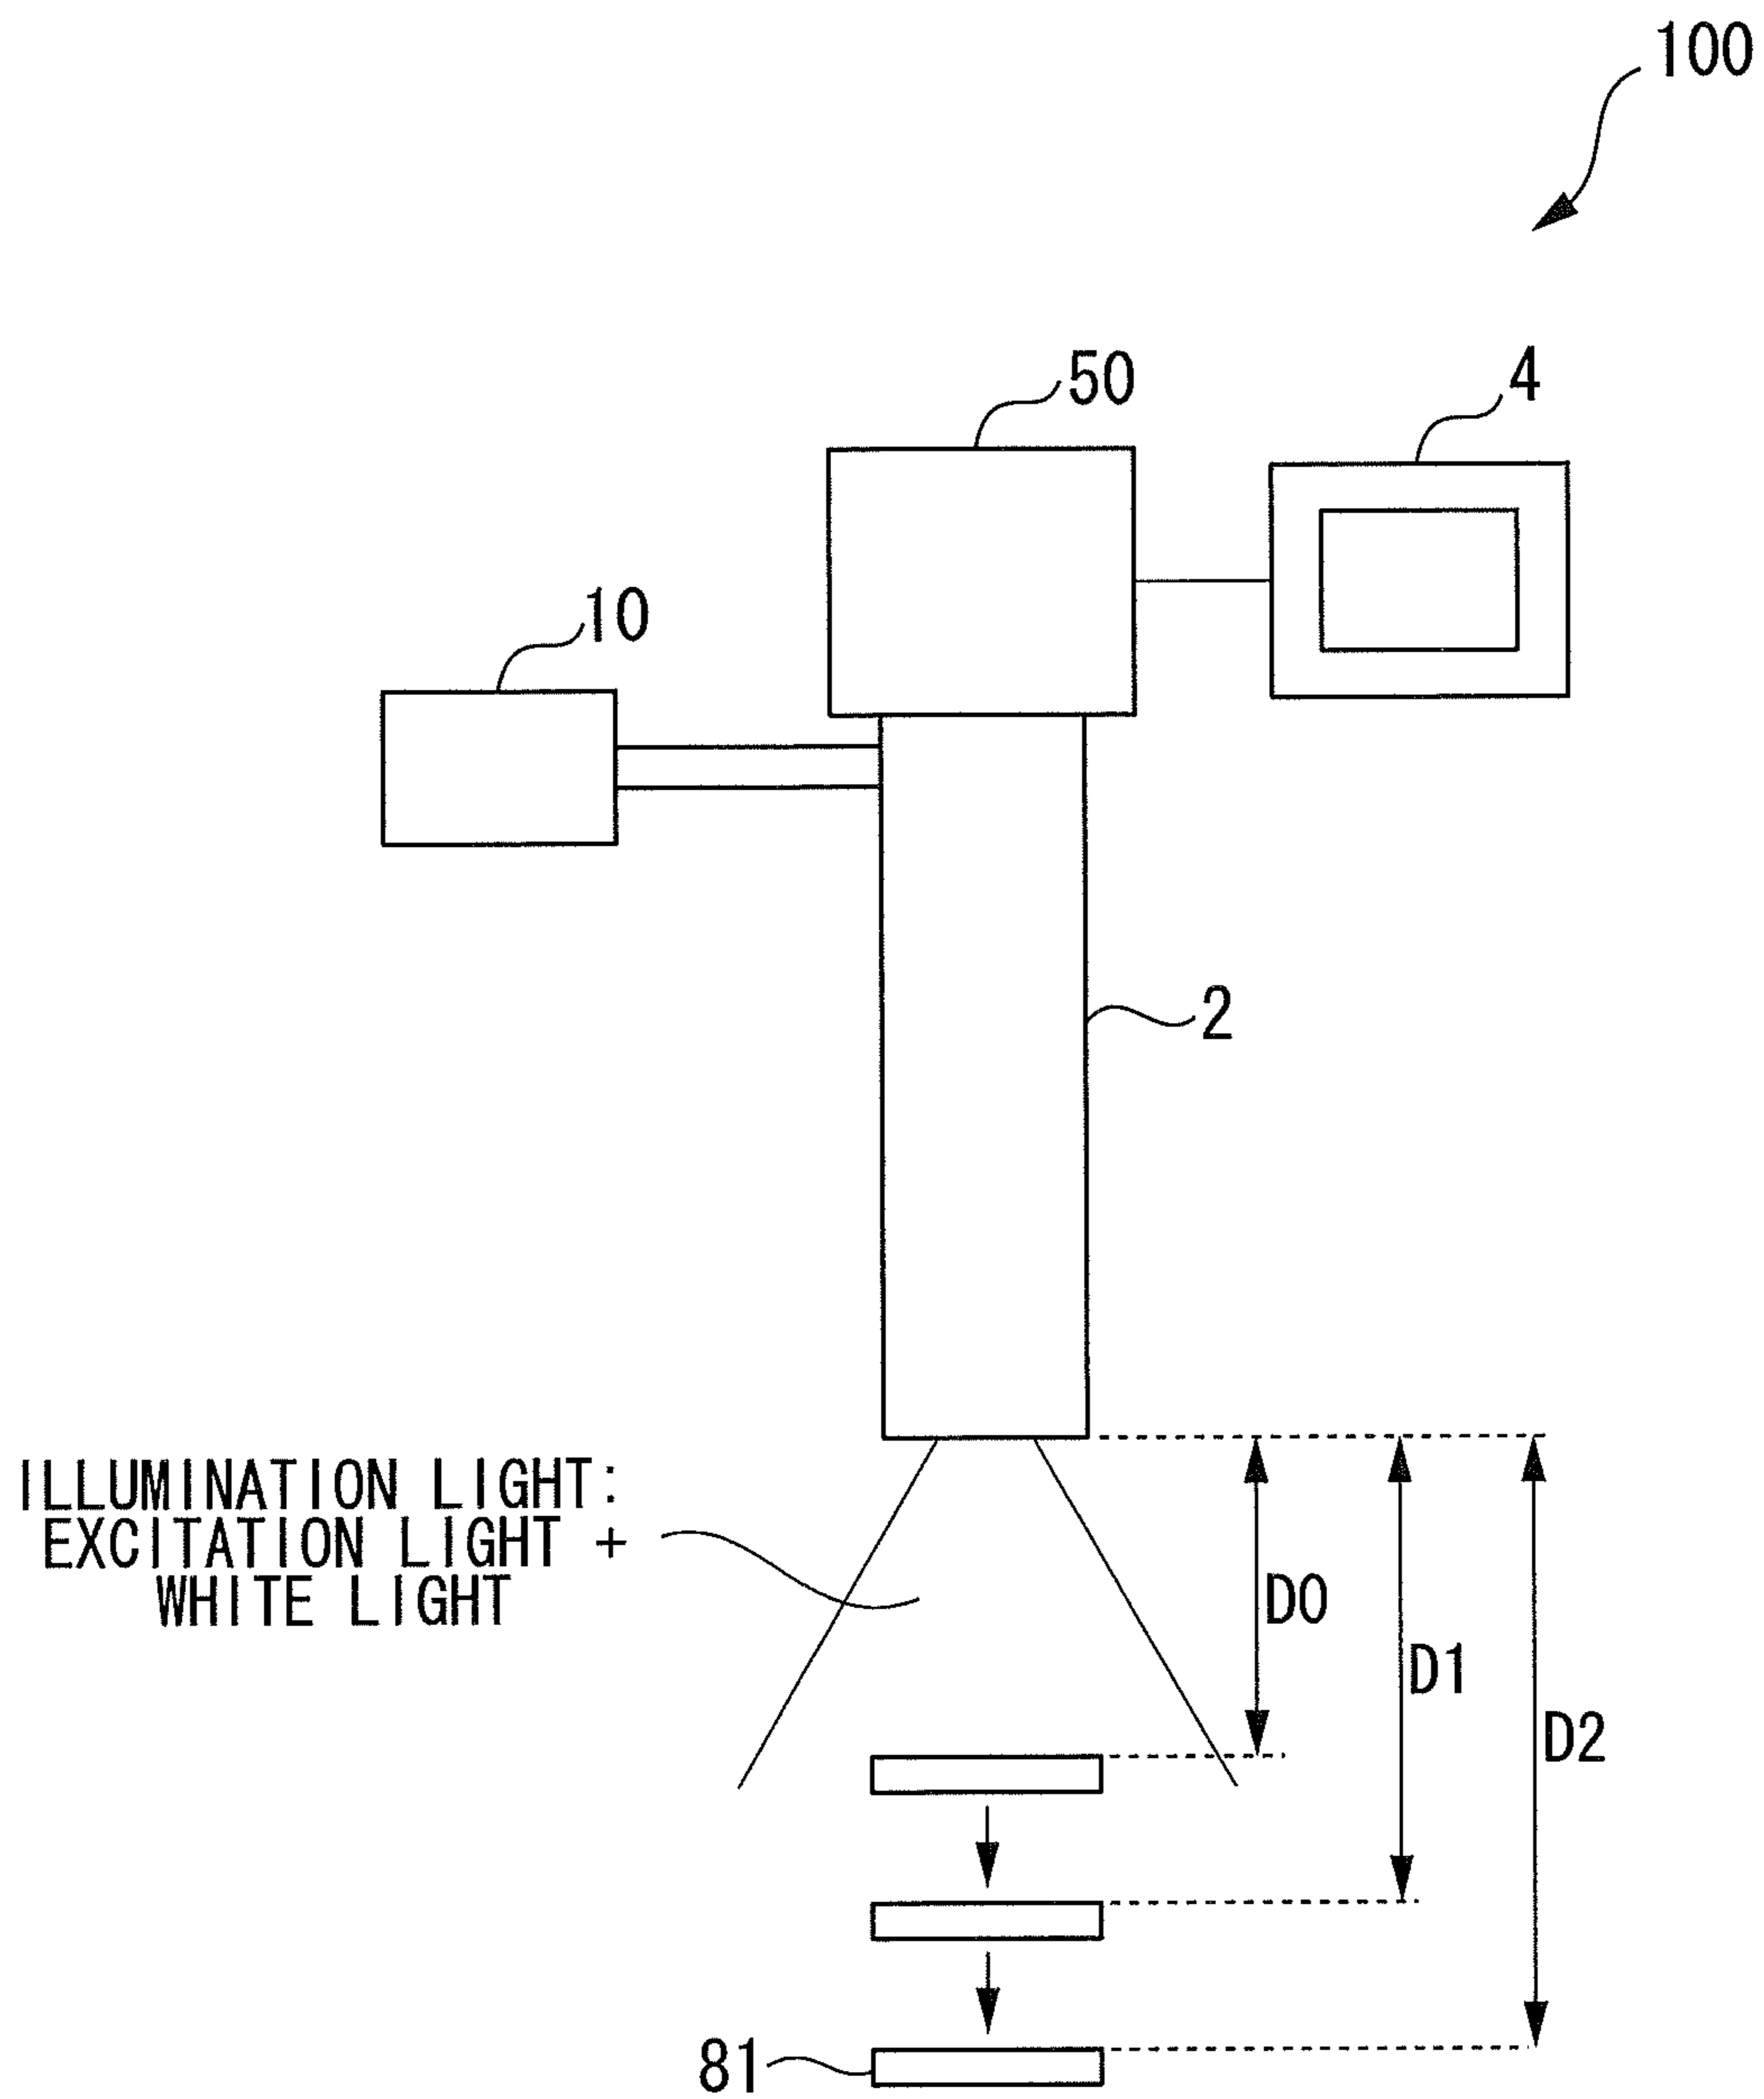


FIG. 3

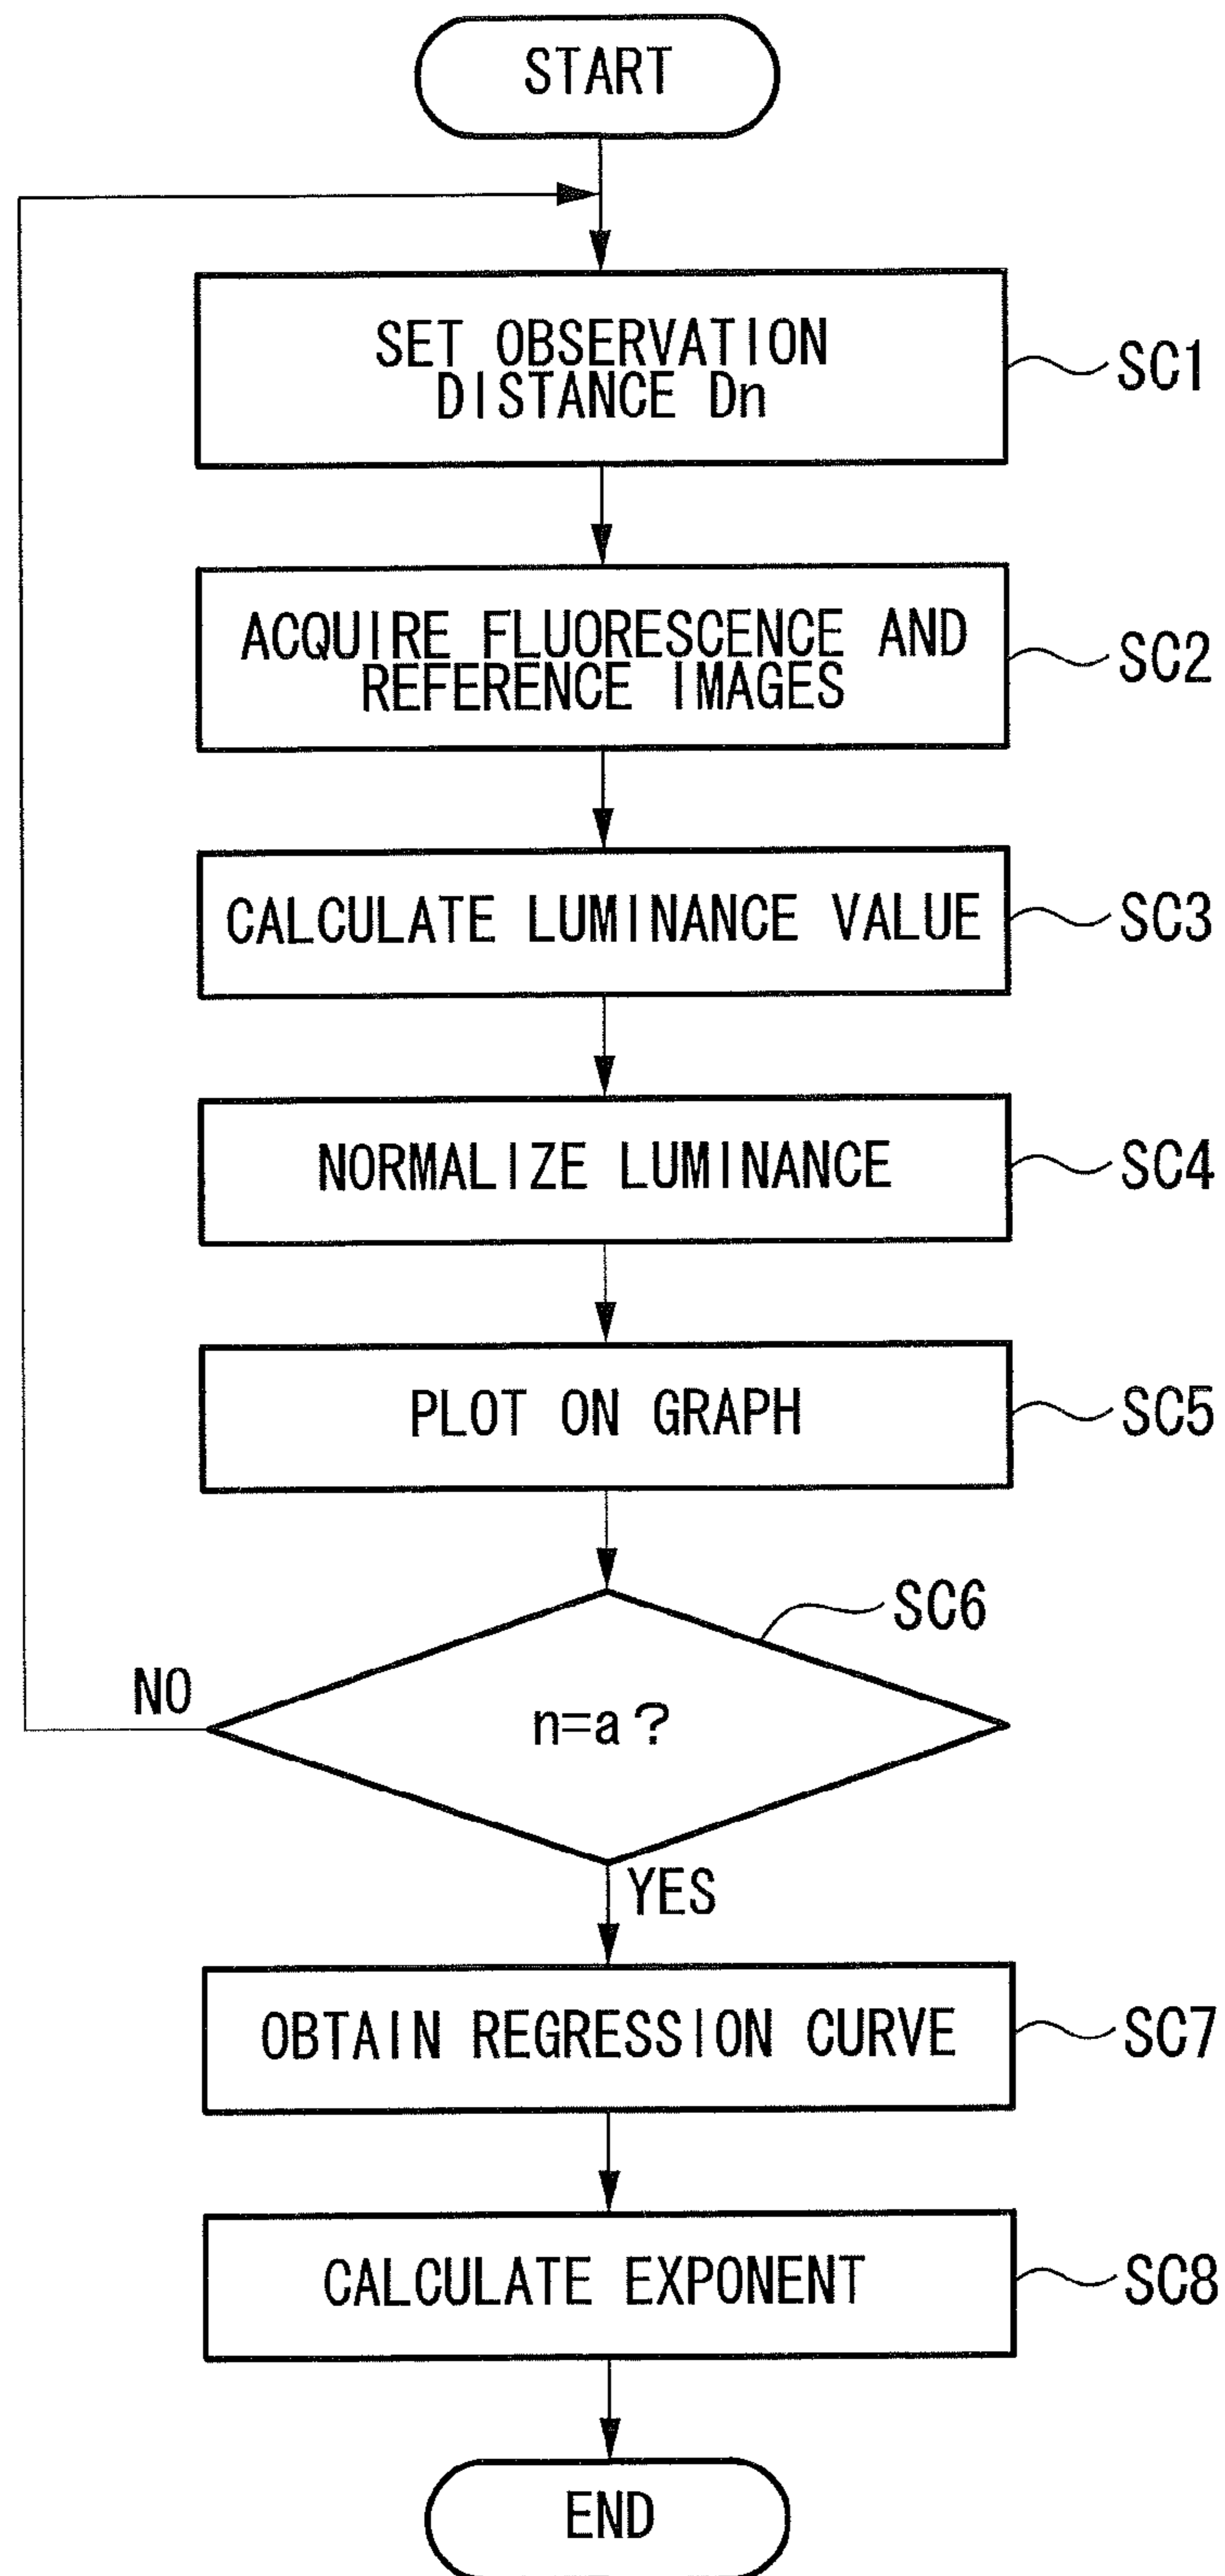


FIG. 4A

D0 IMAGE

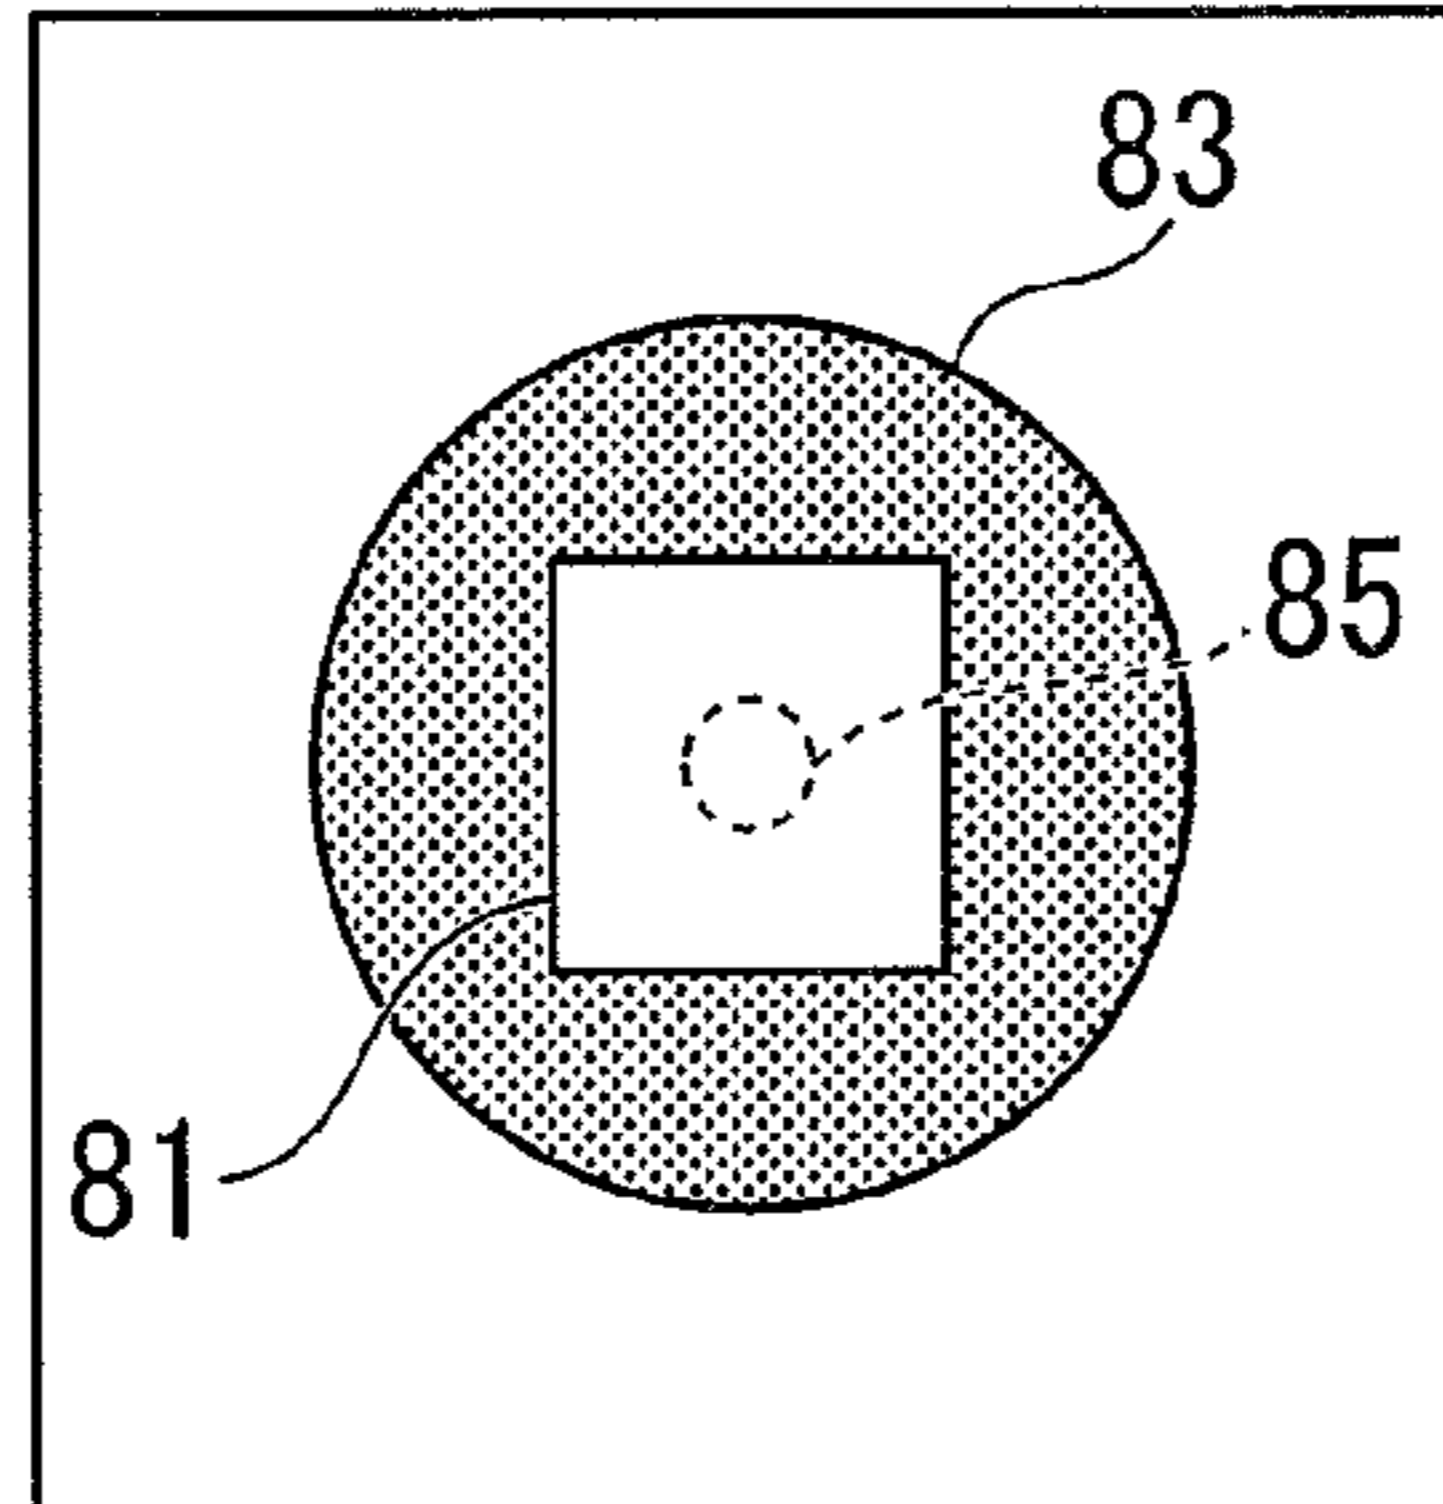


FIG. 4B

D1 IMAGE

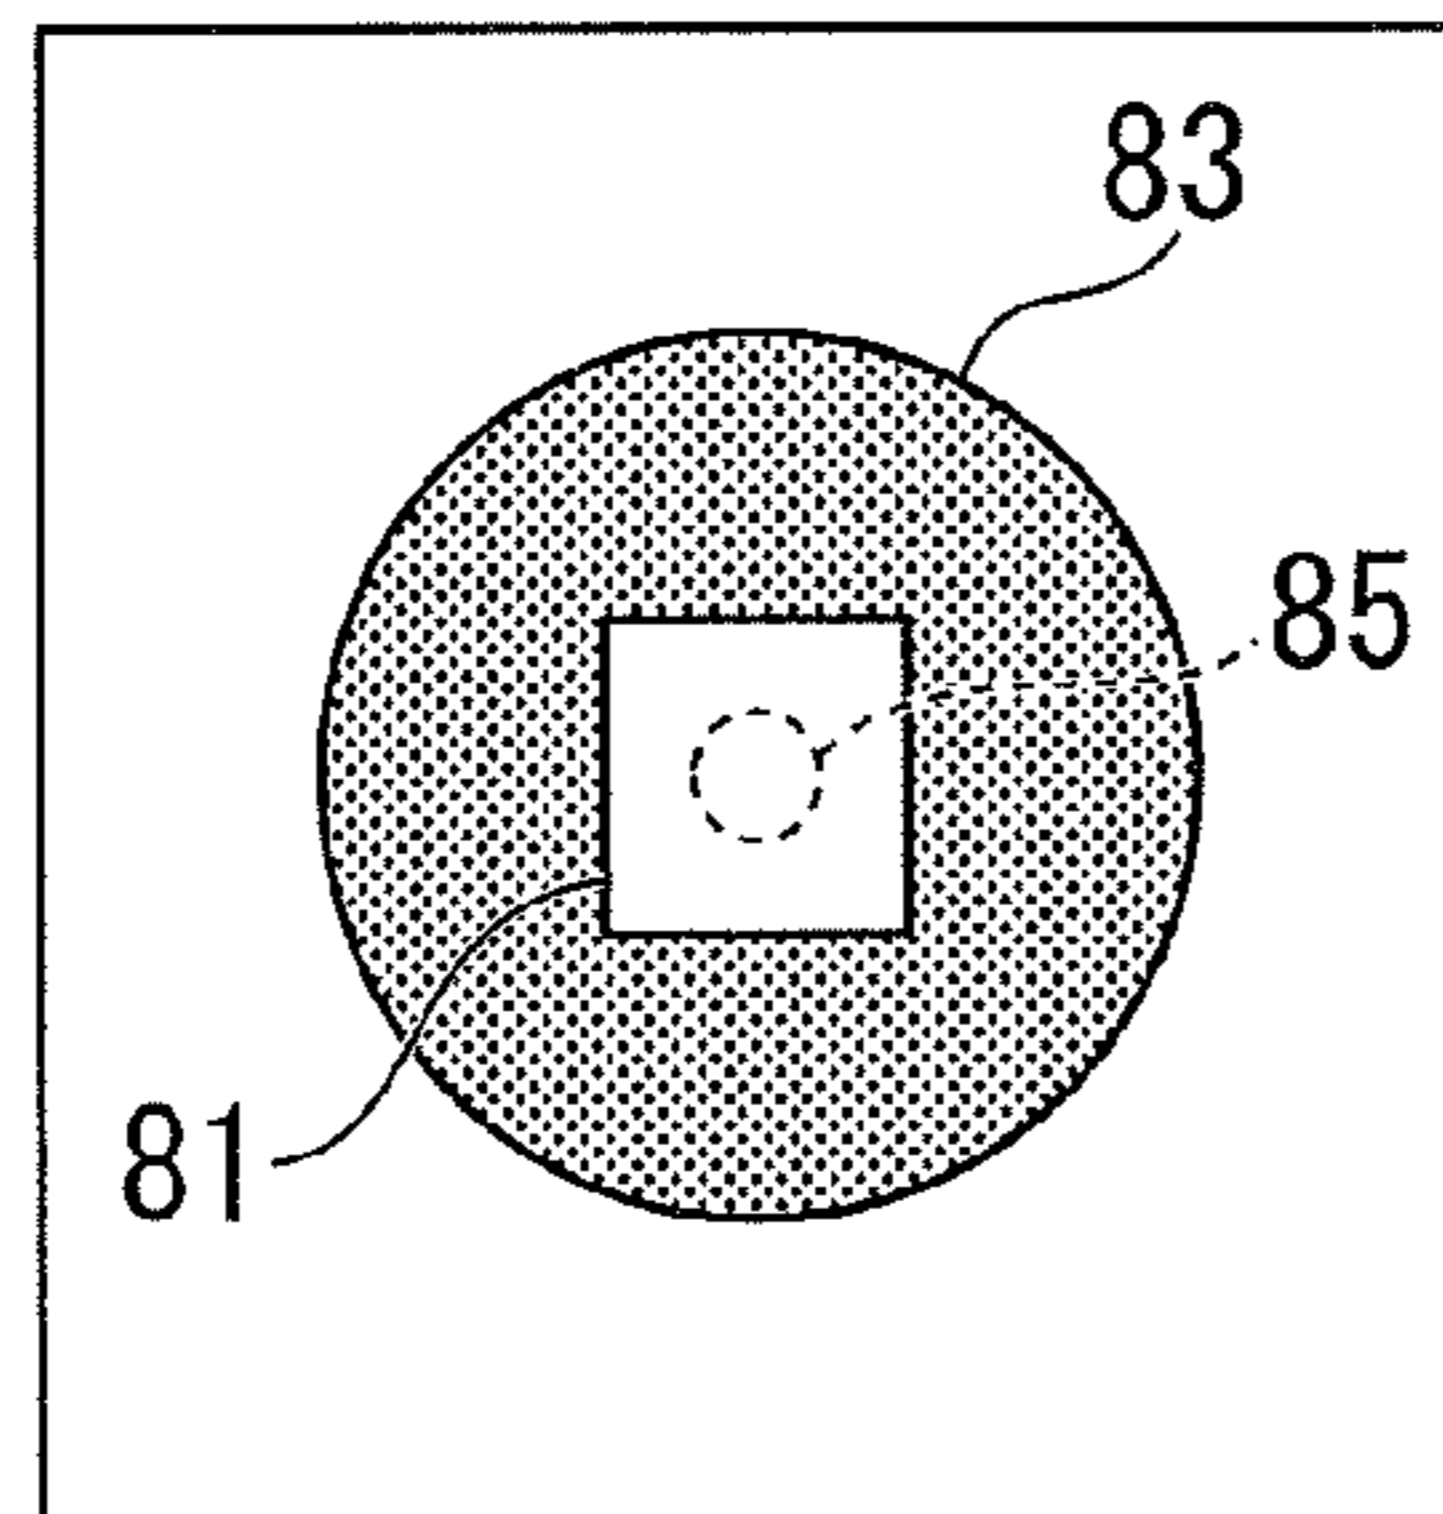


FIG. 4C

D2 IMAGE

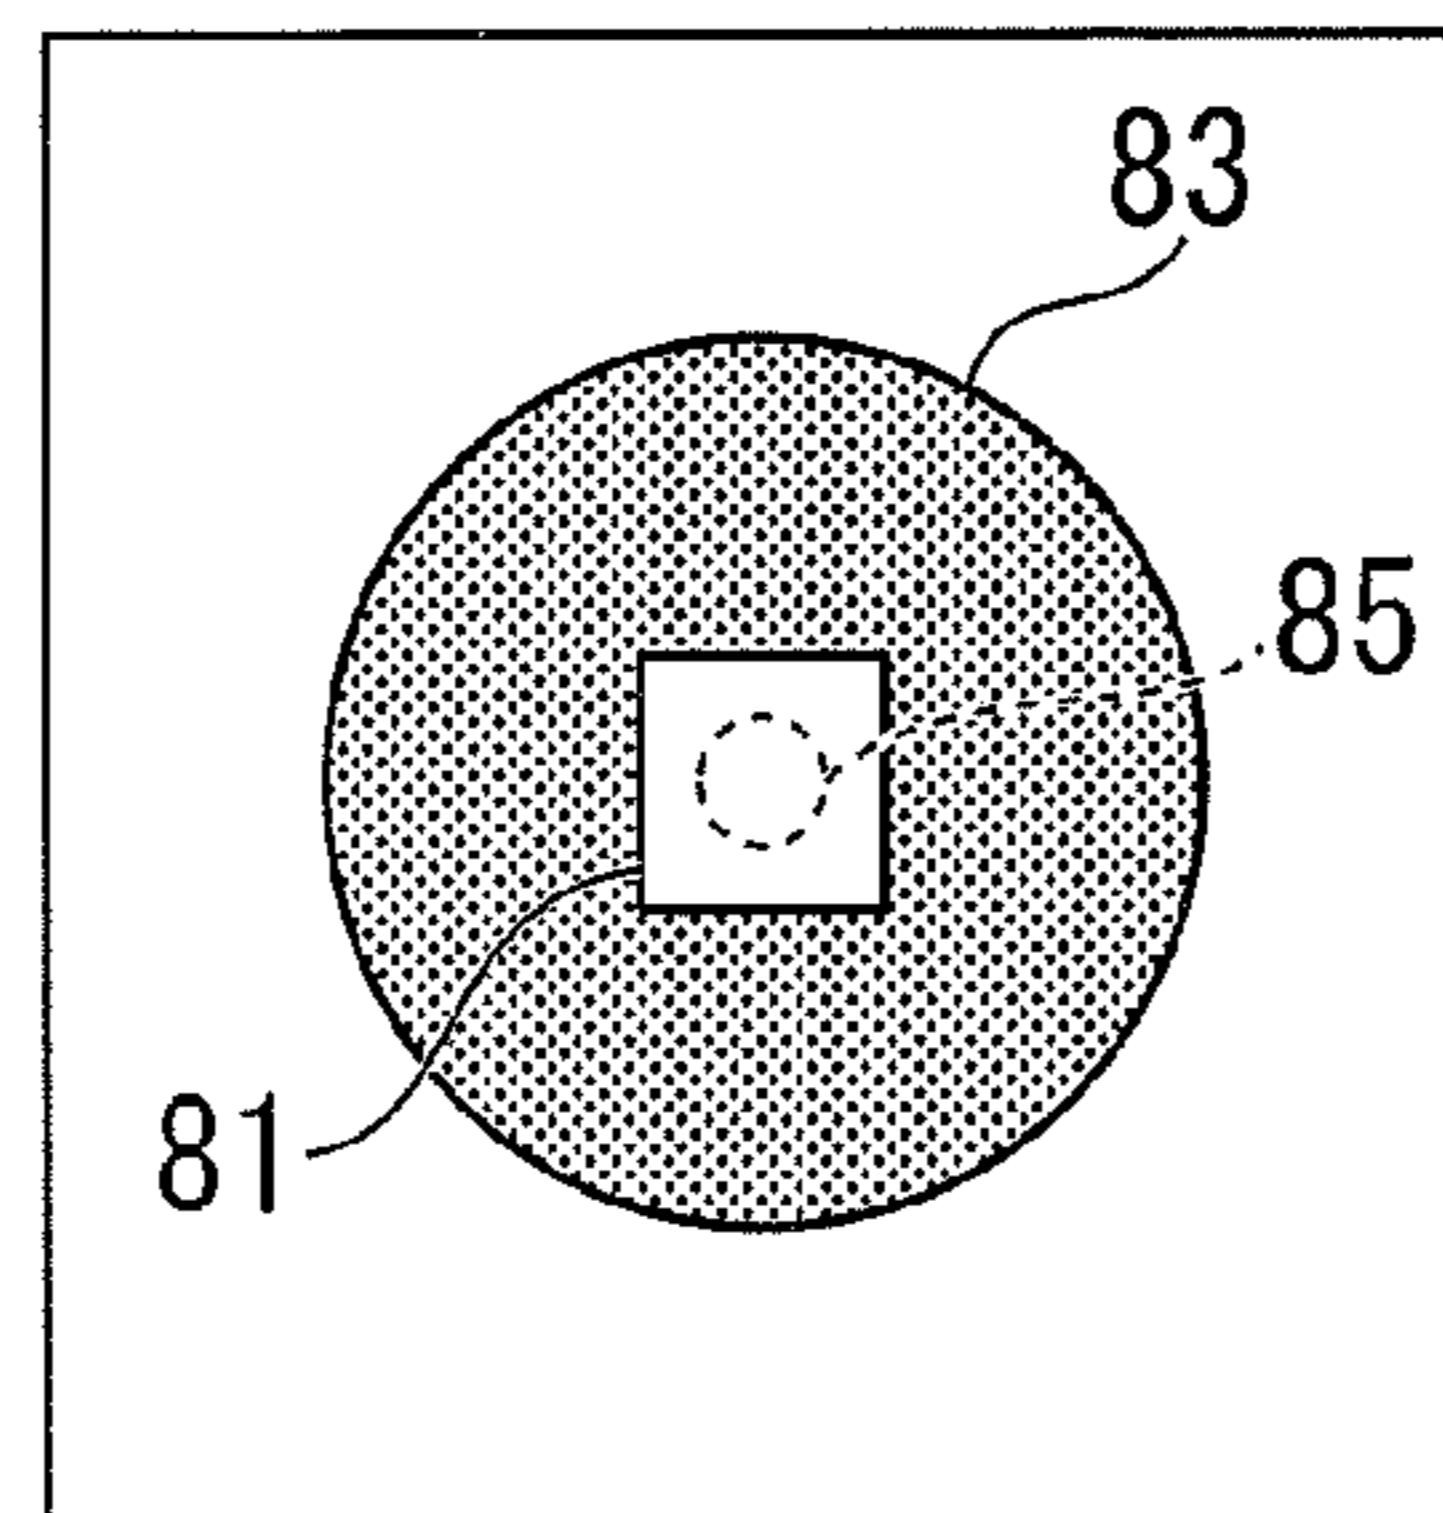


FIG. 5A

D0 IMAGE

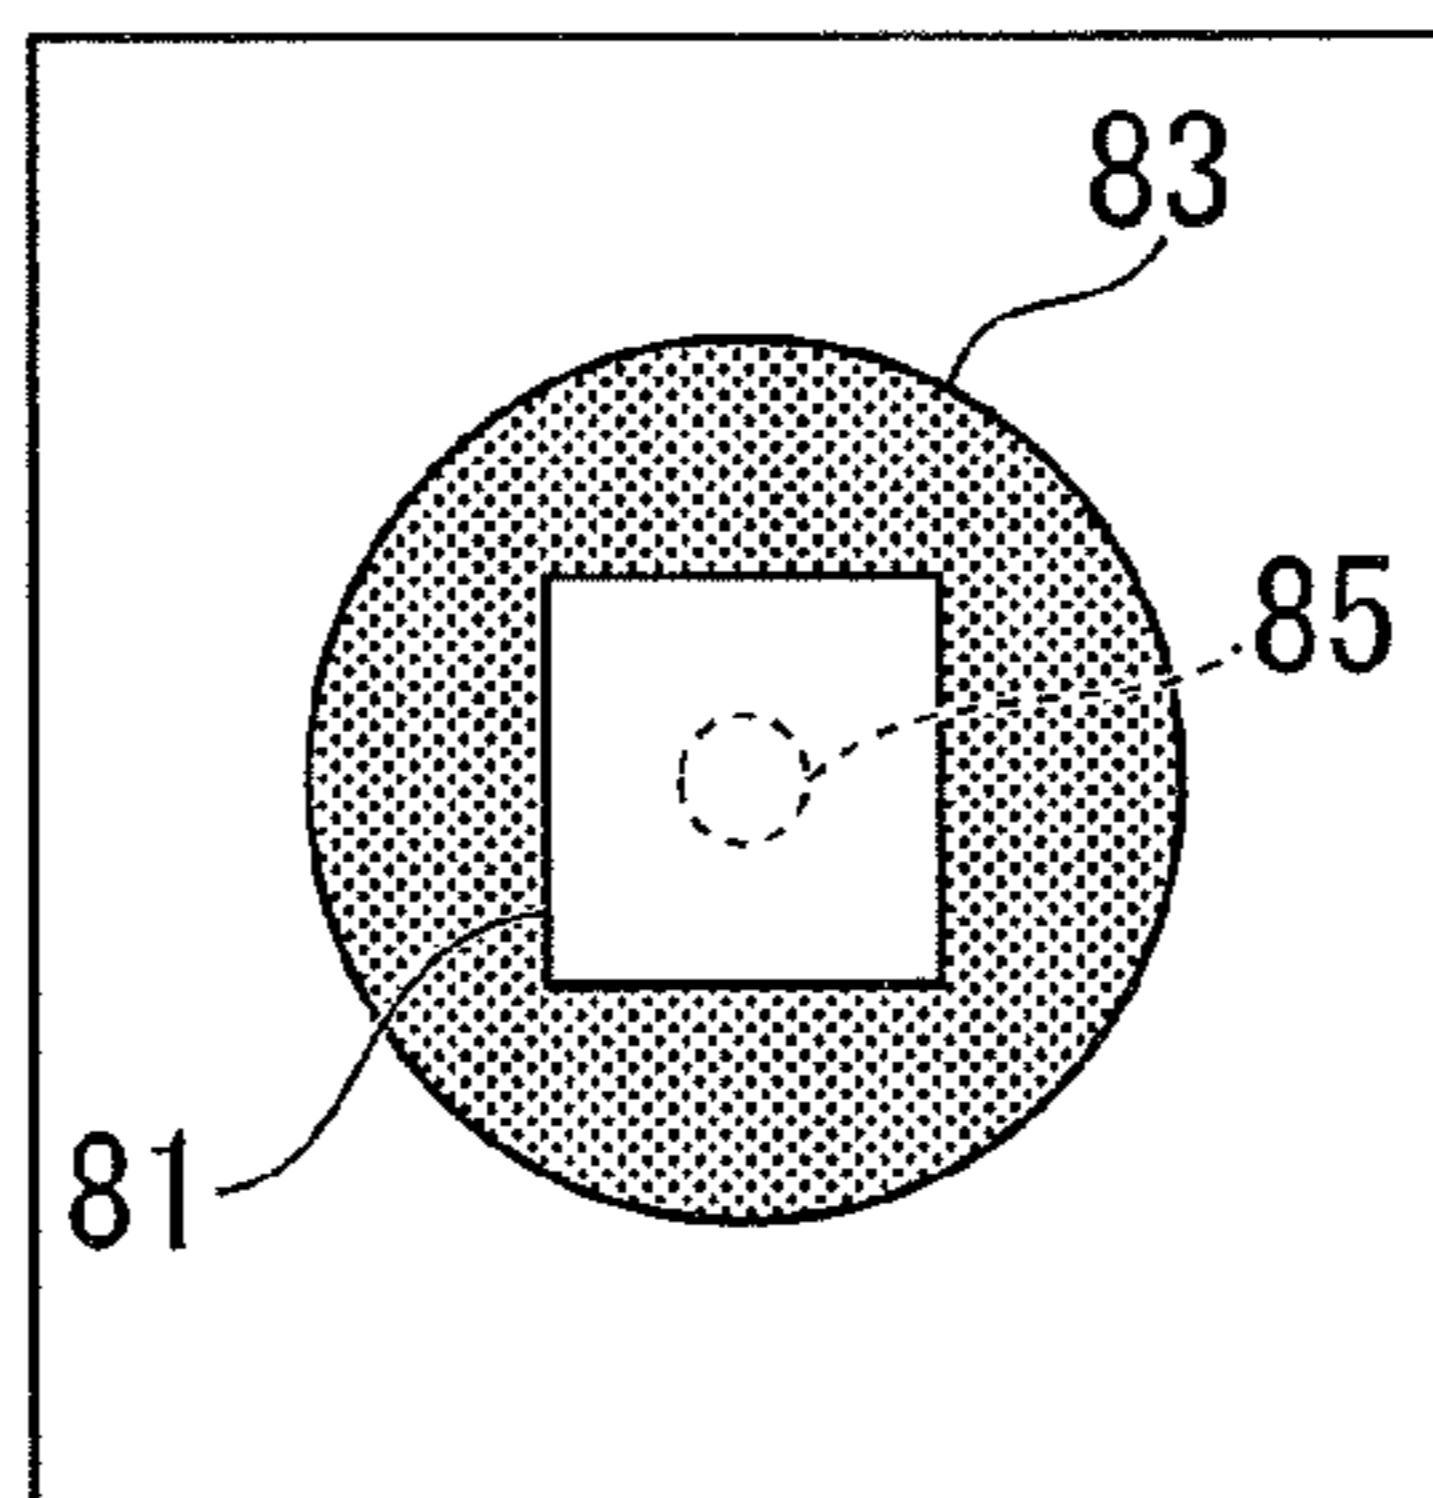


FIG. 5B

D1 IMAGE

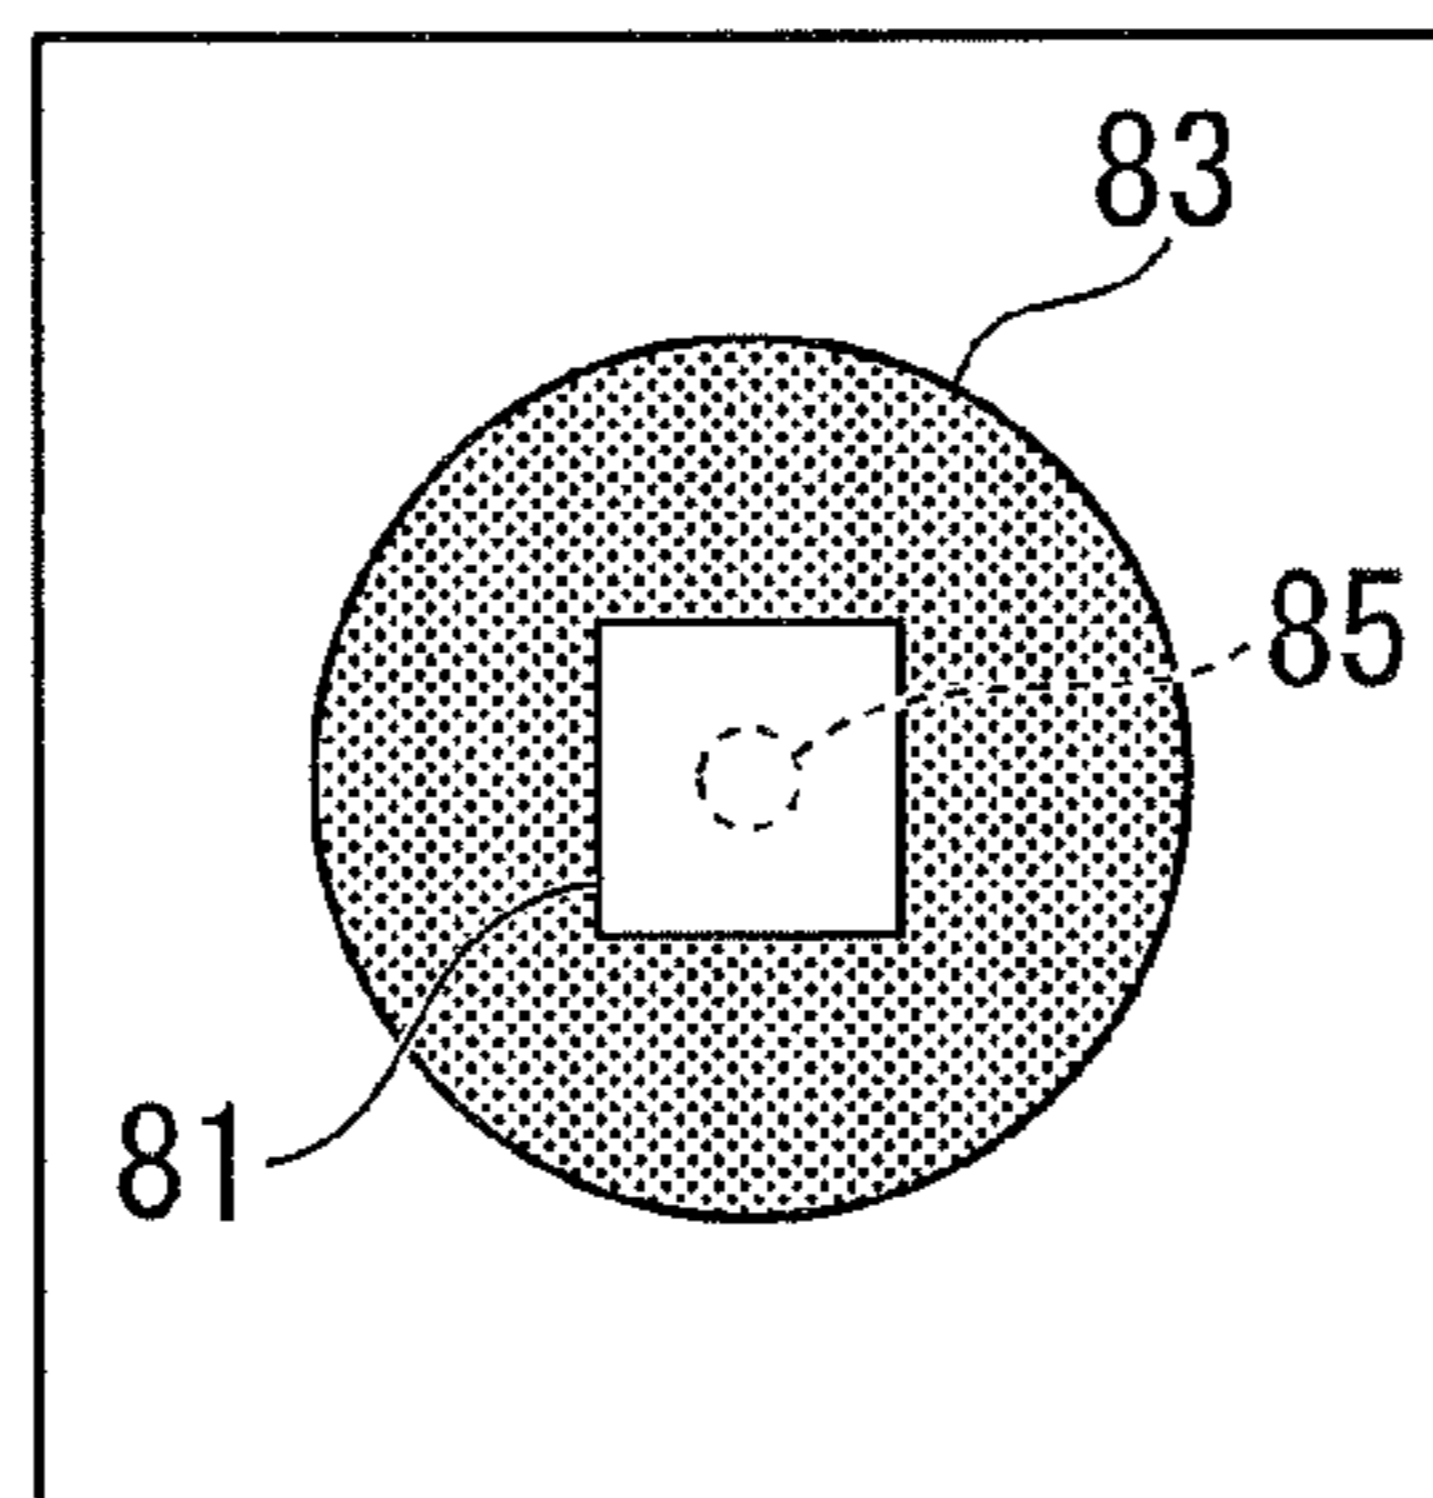


FIG. 5C

D2 IMAGE

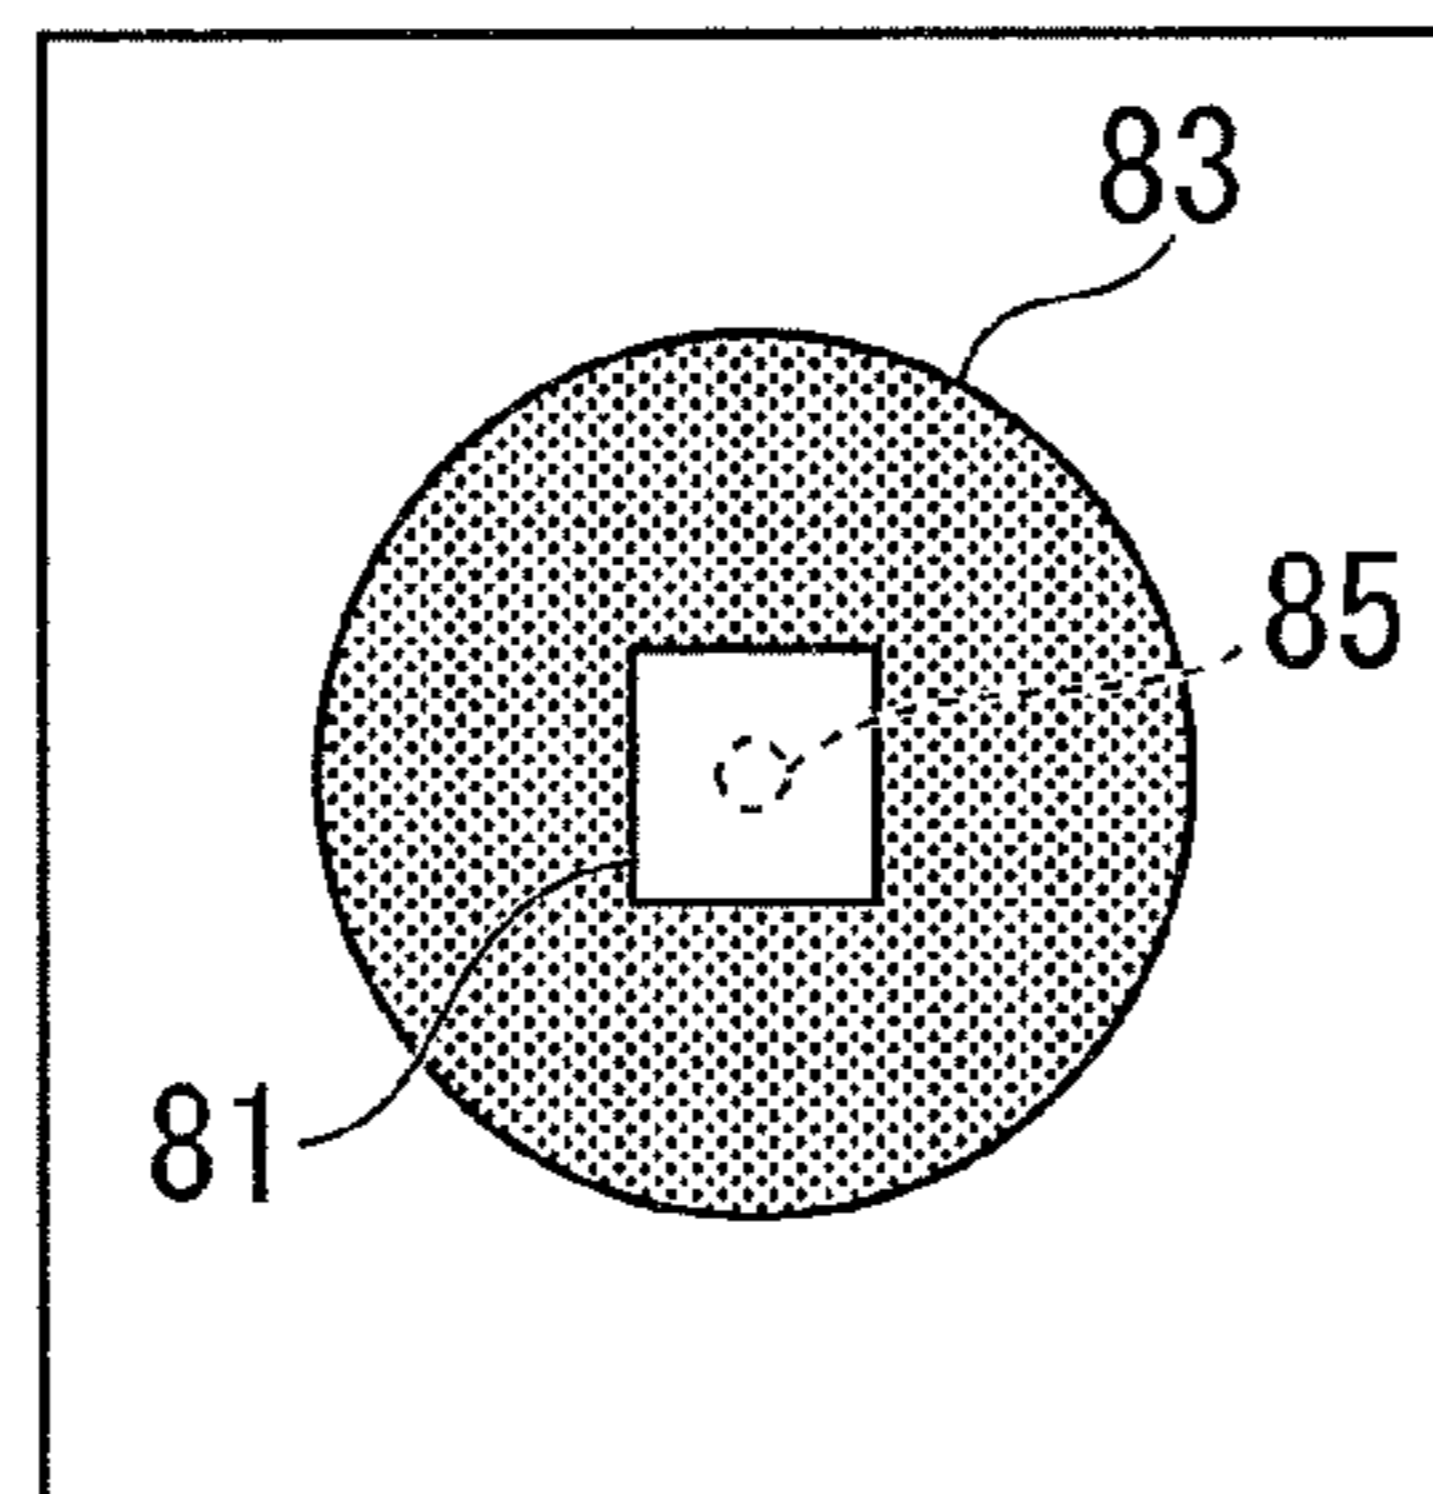


FIG. 6

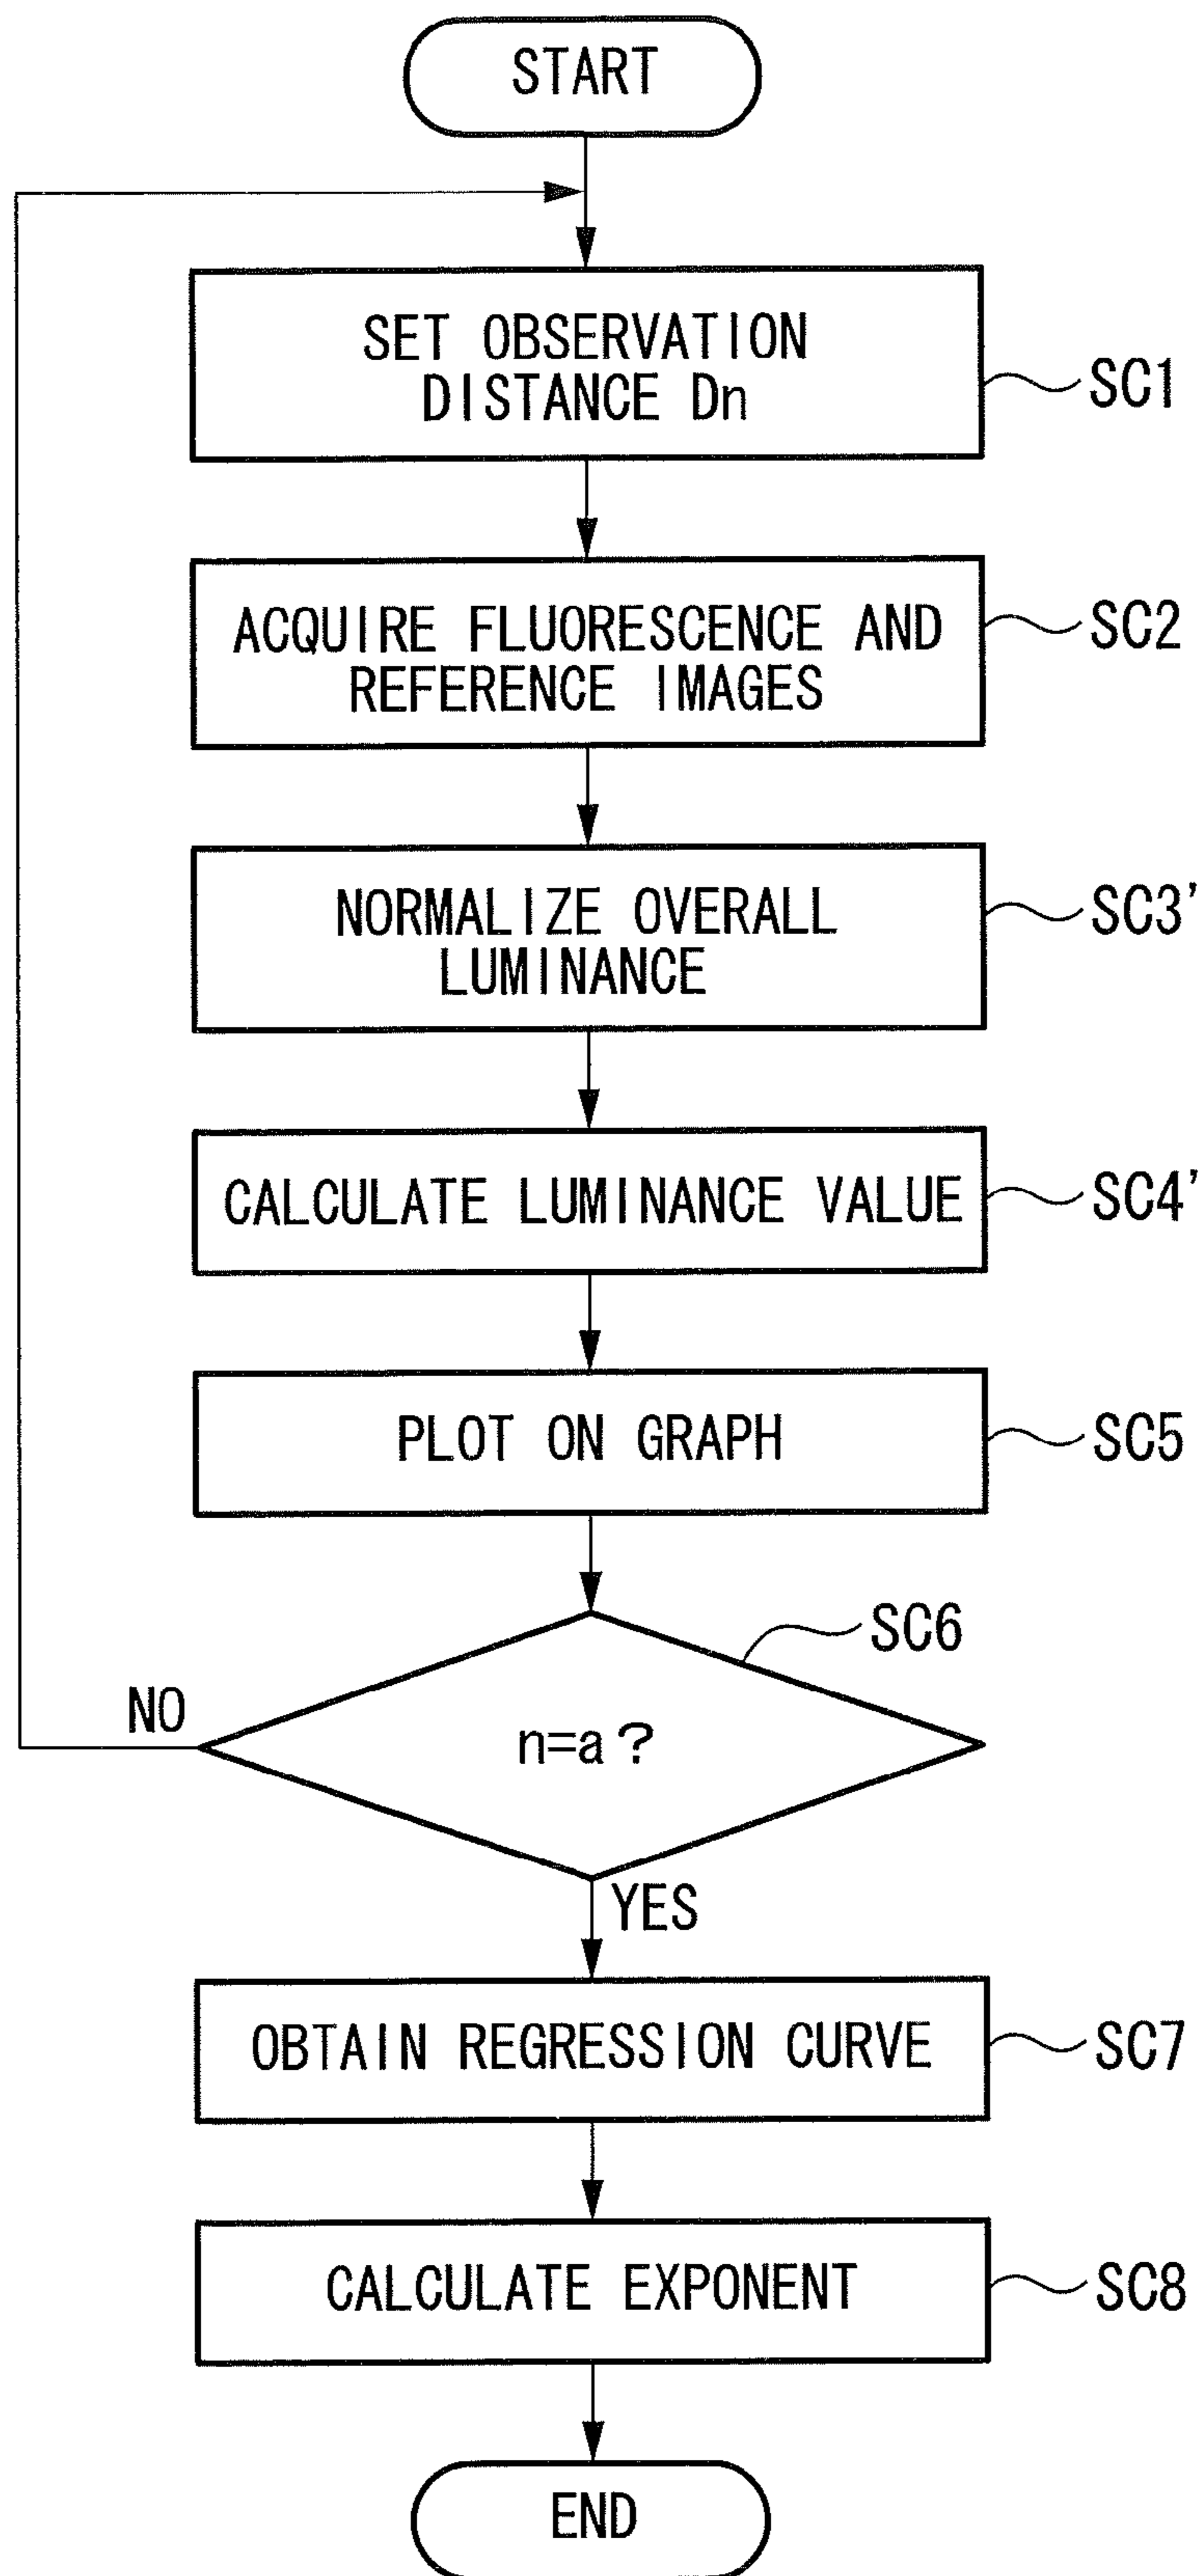


FIG. 7

CORRECTED FLUORESCENCE IMAGE LUMINANCE VALUE	FLUORESCENCE CONCENTRATION (nM)
0	0
1	1
⋮	⋮
4095	1000

87


FIG. 8

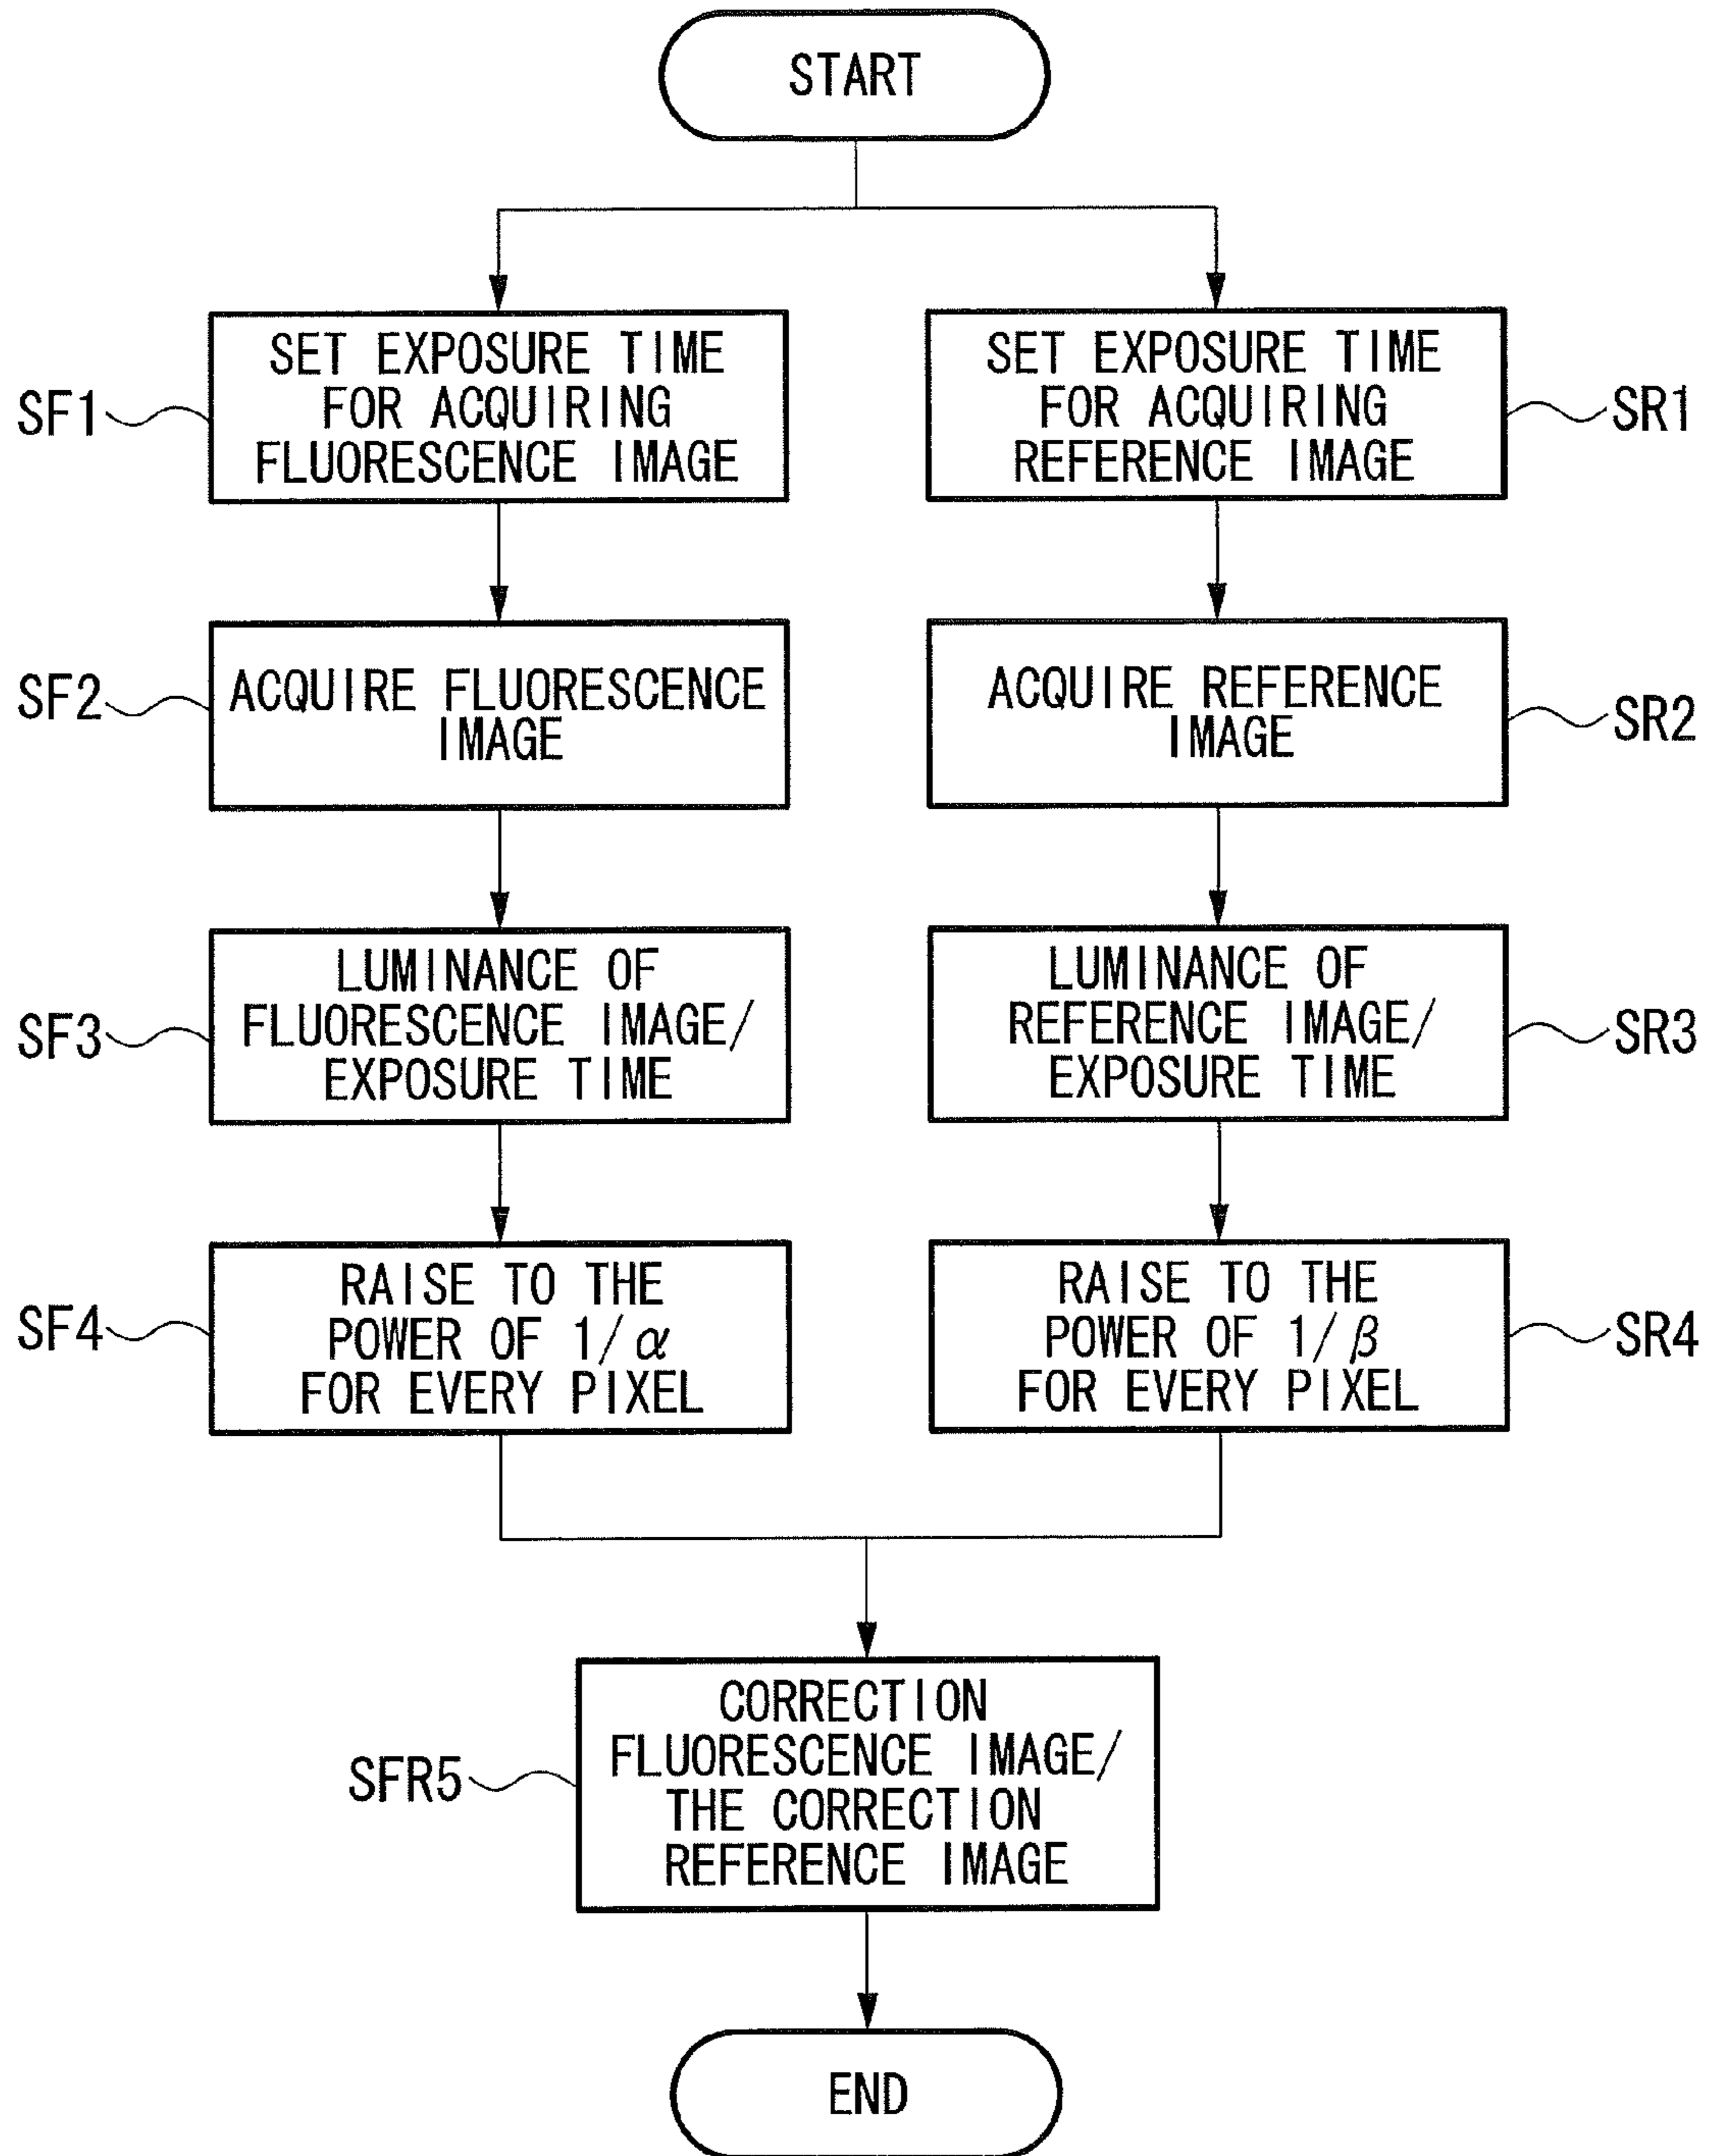


FIG. 9A

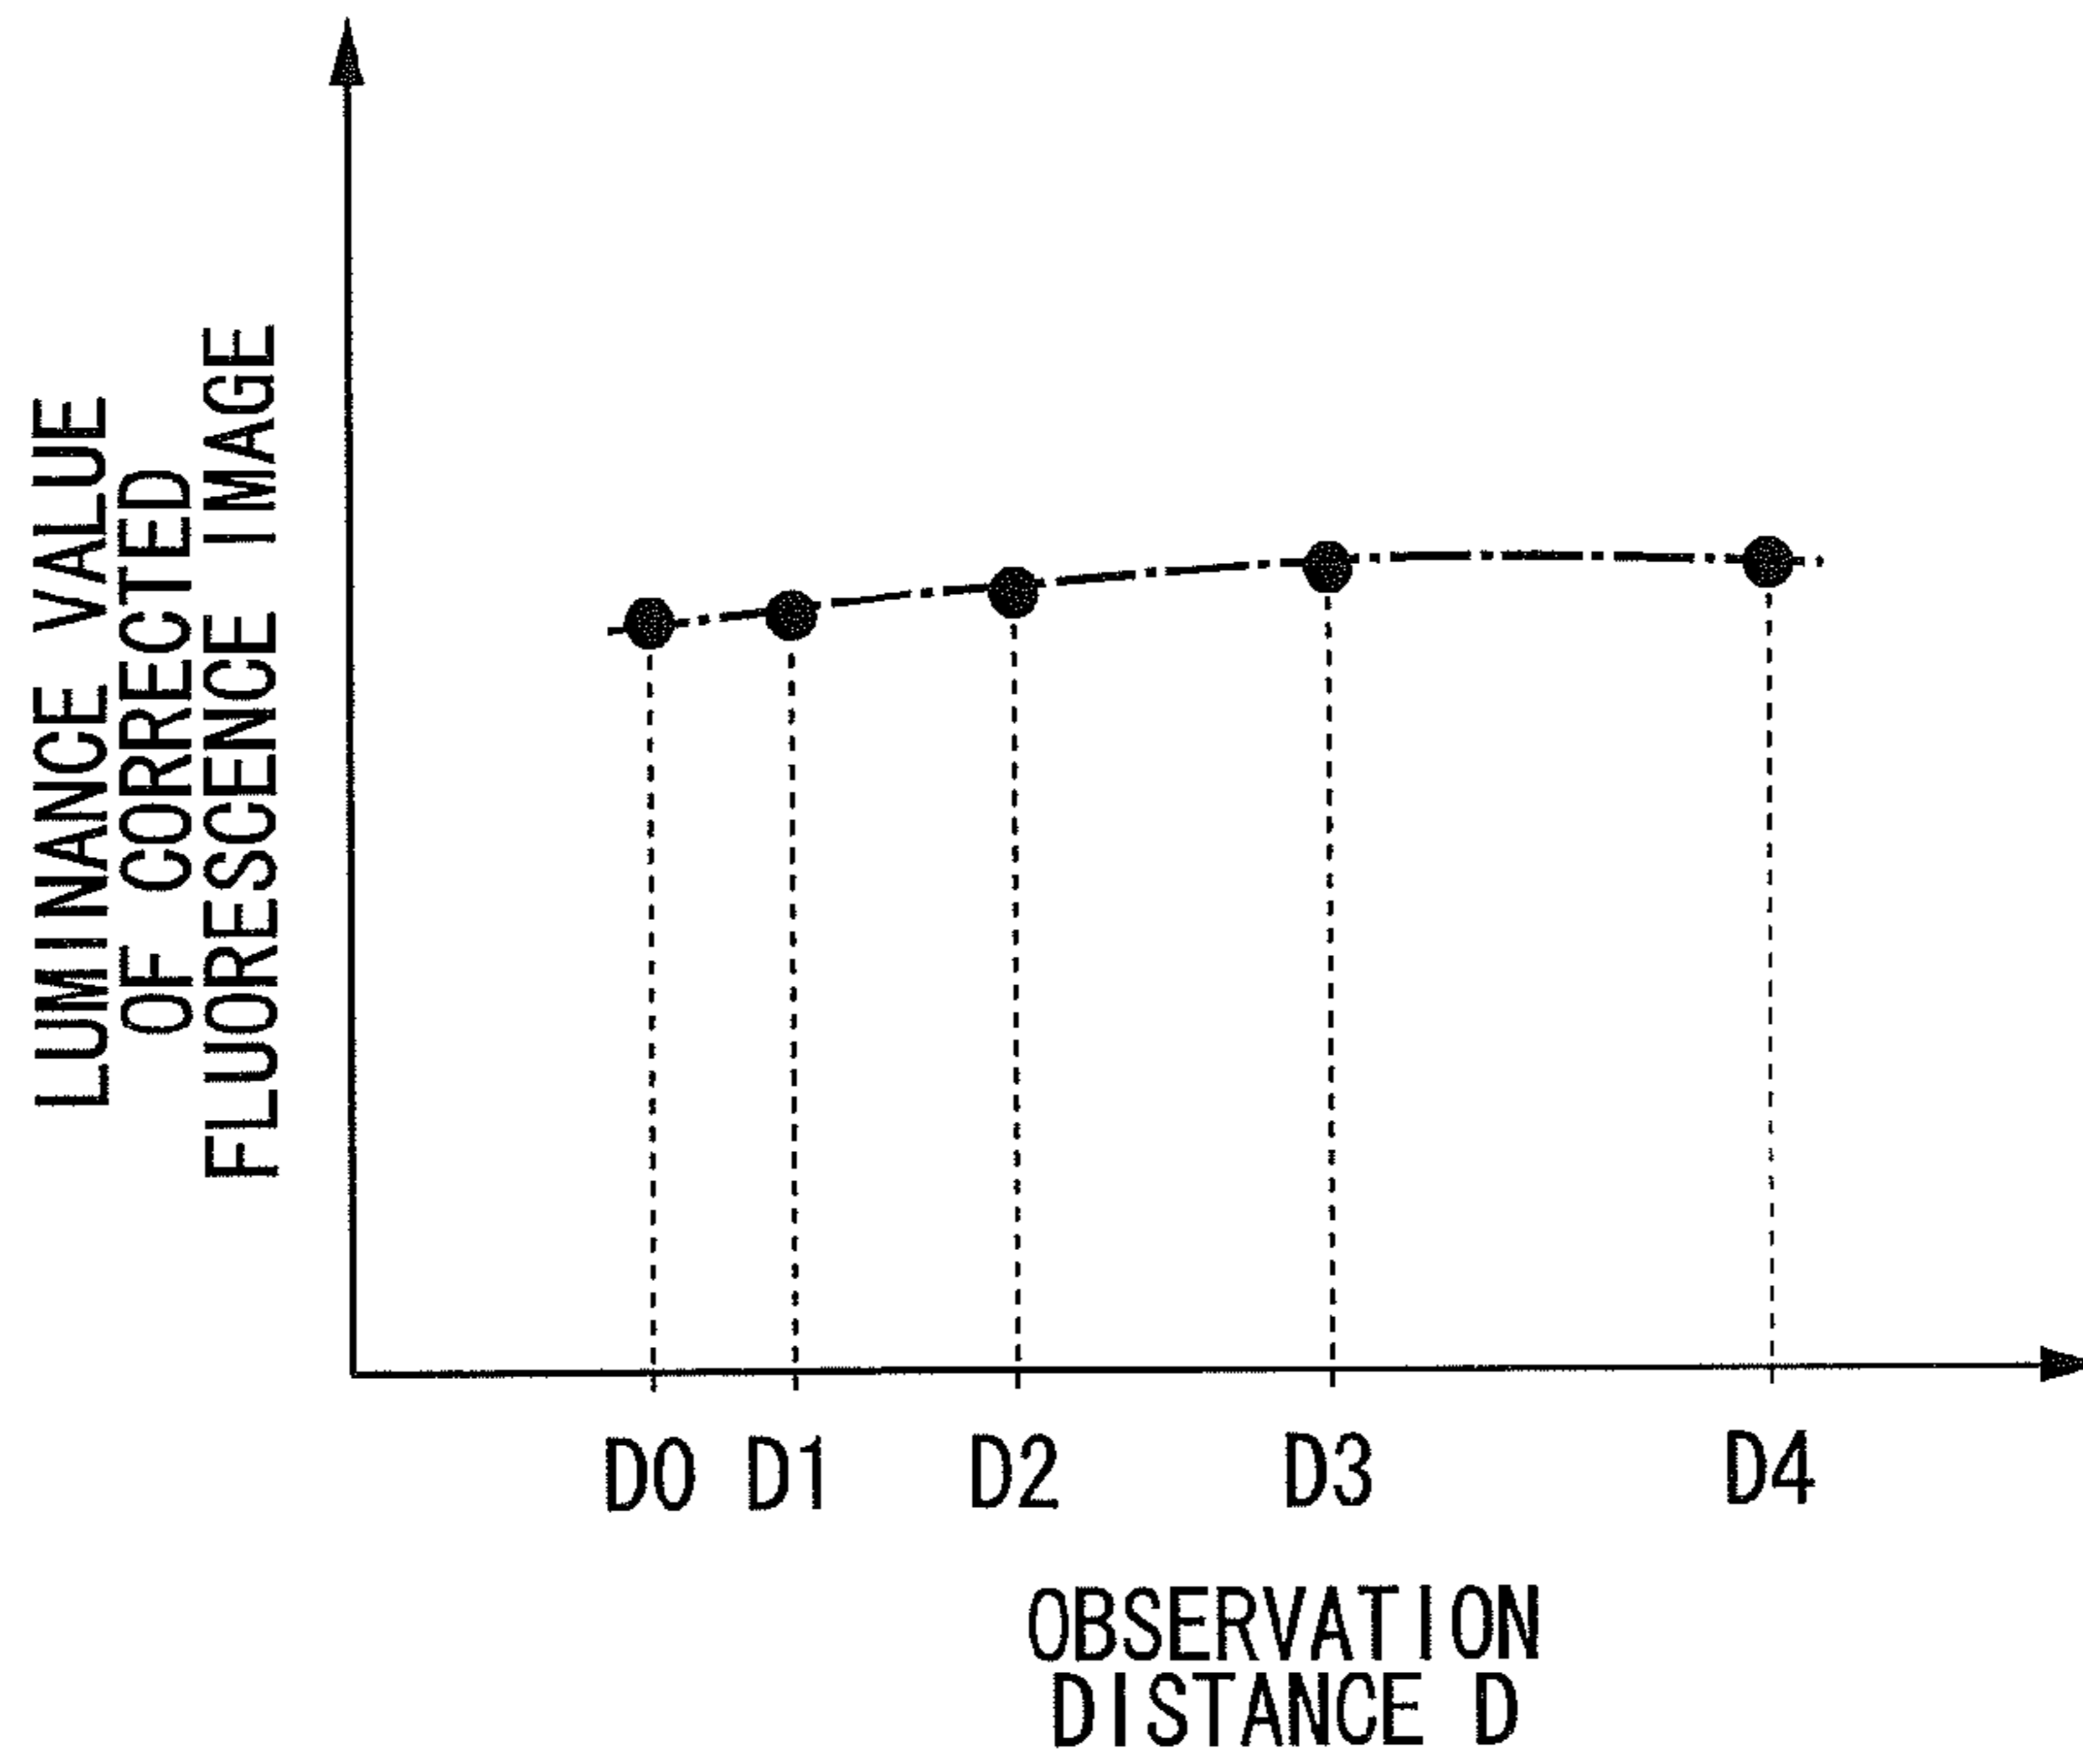


FIG. 9B

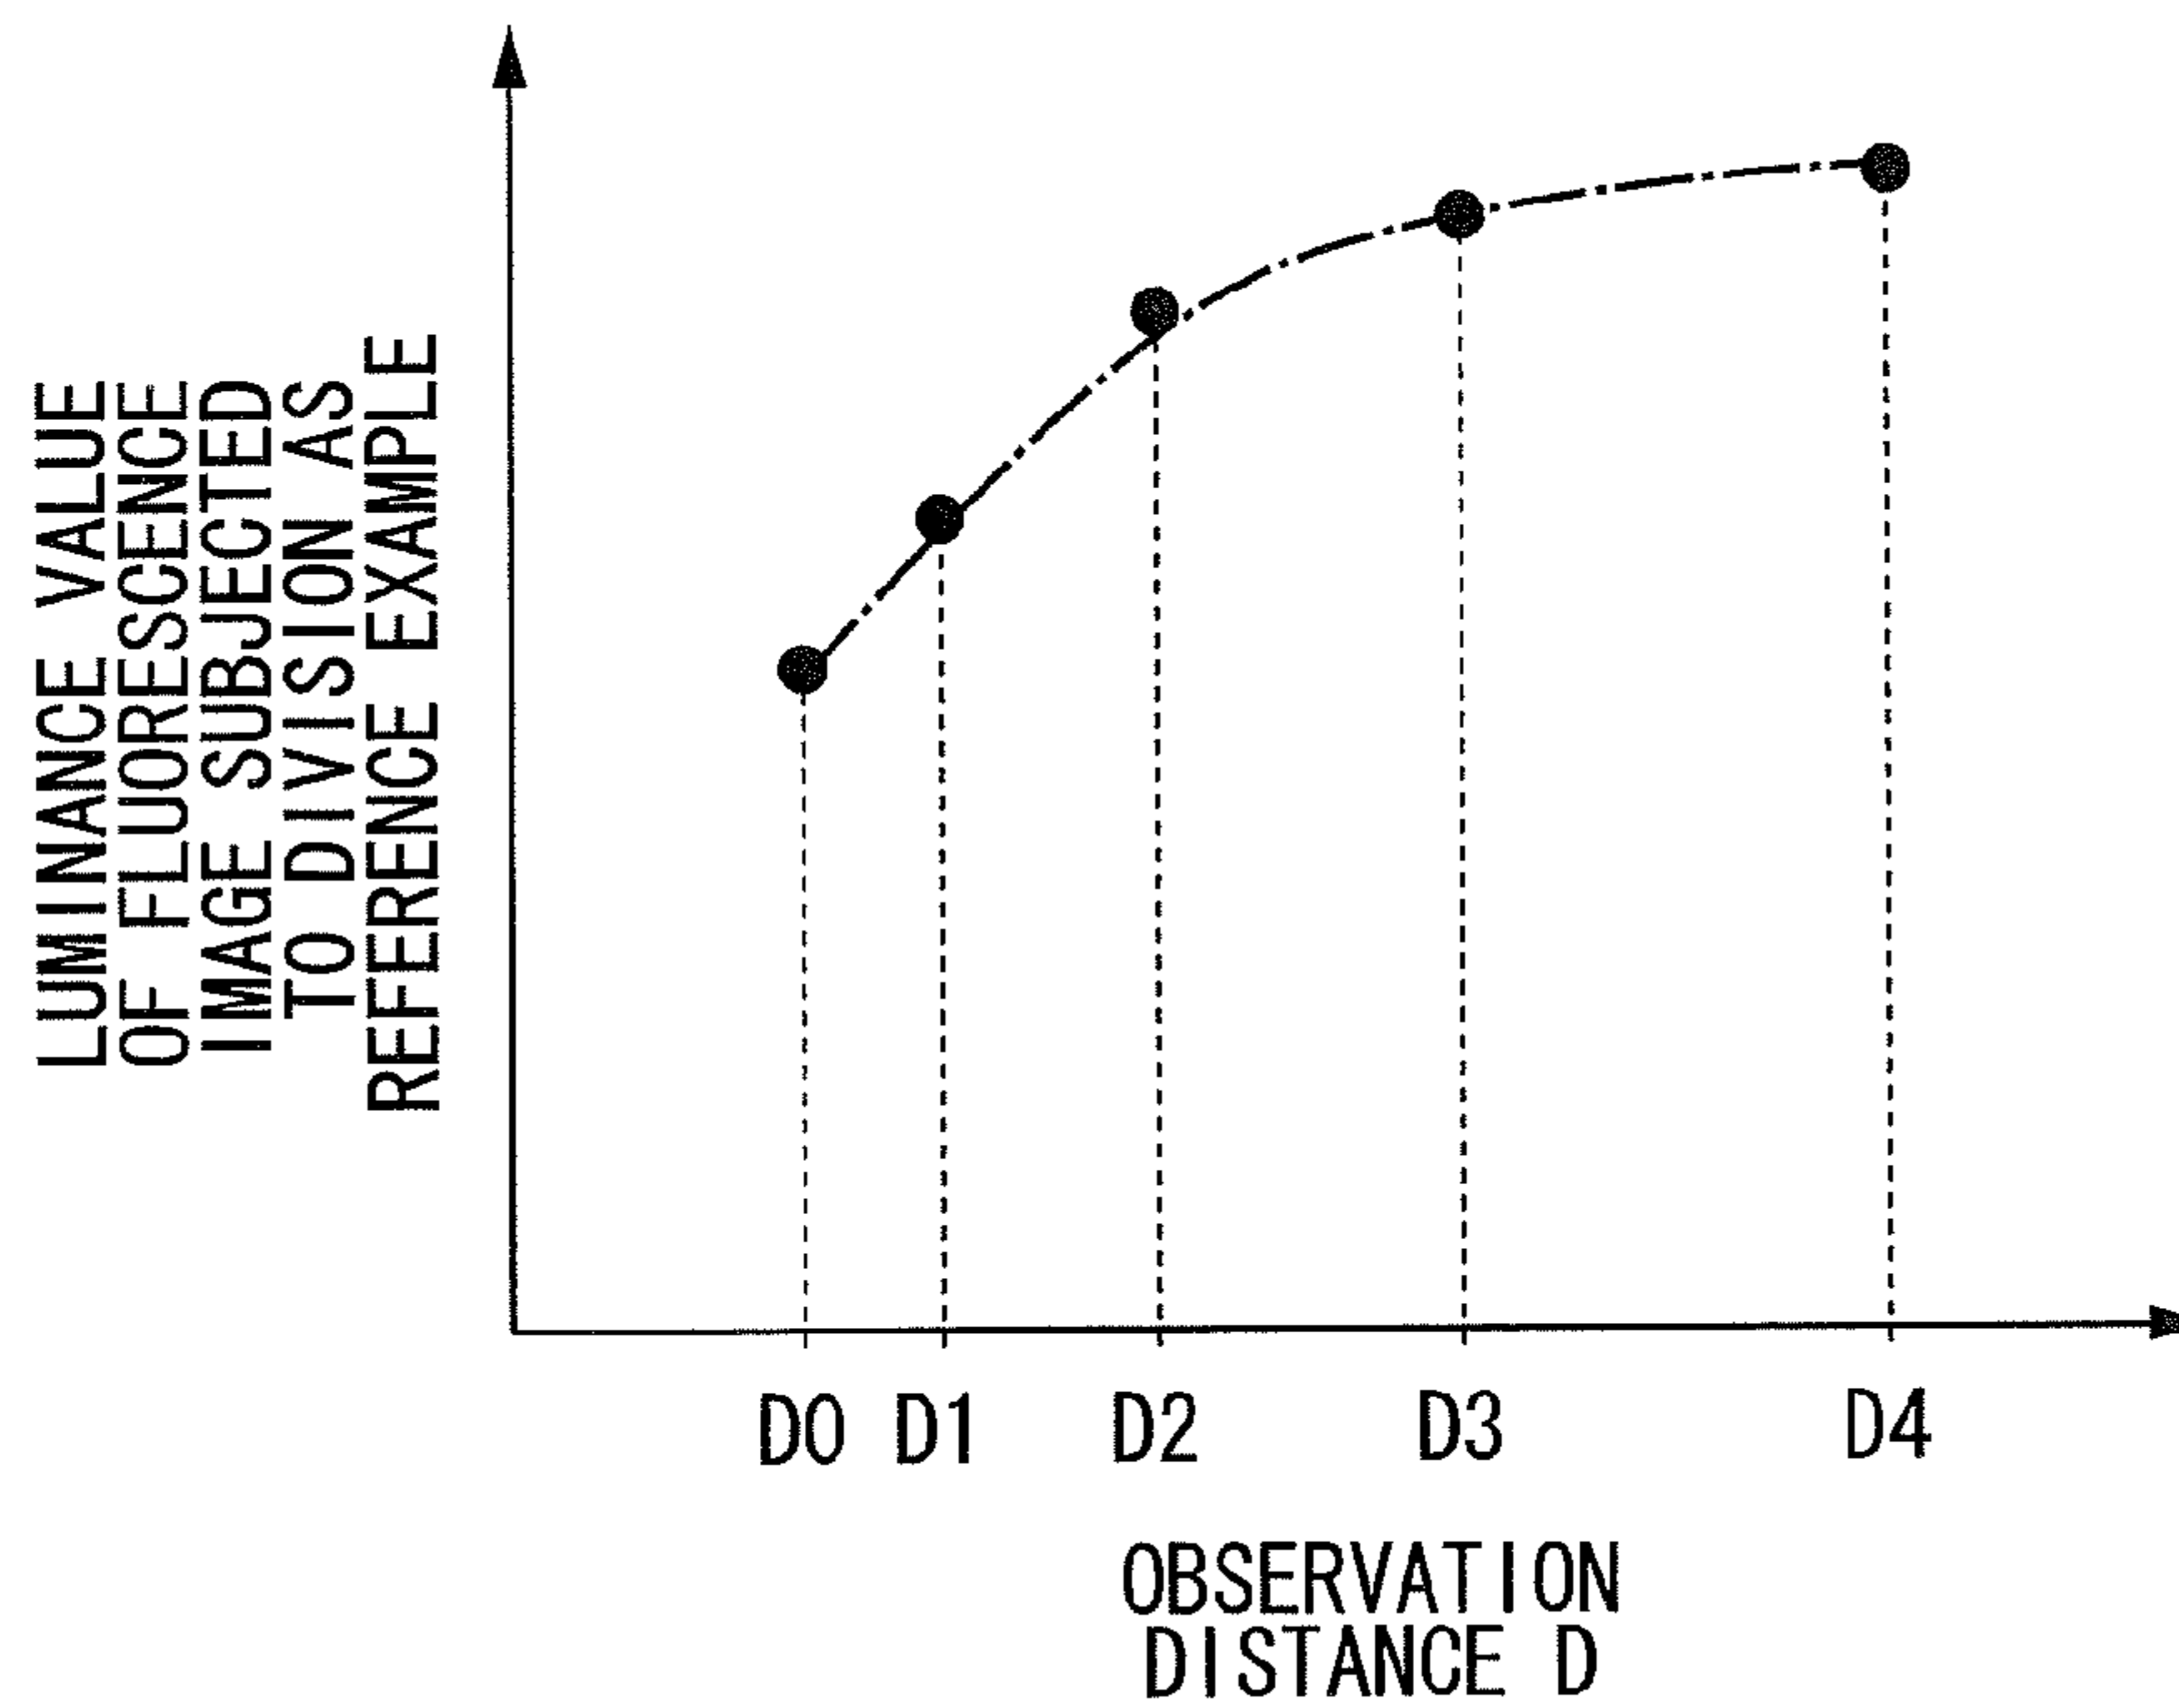
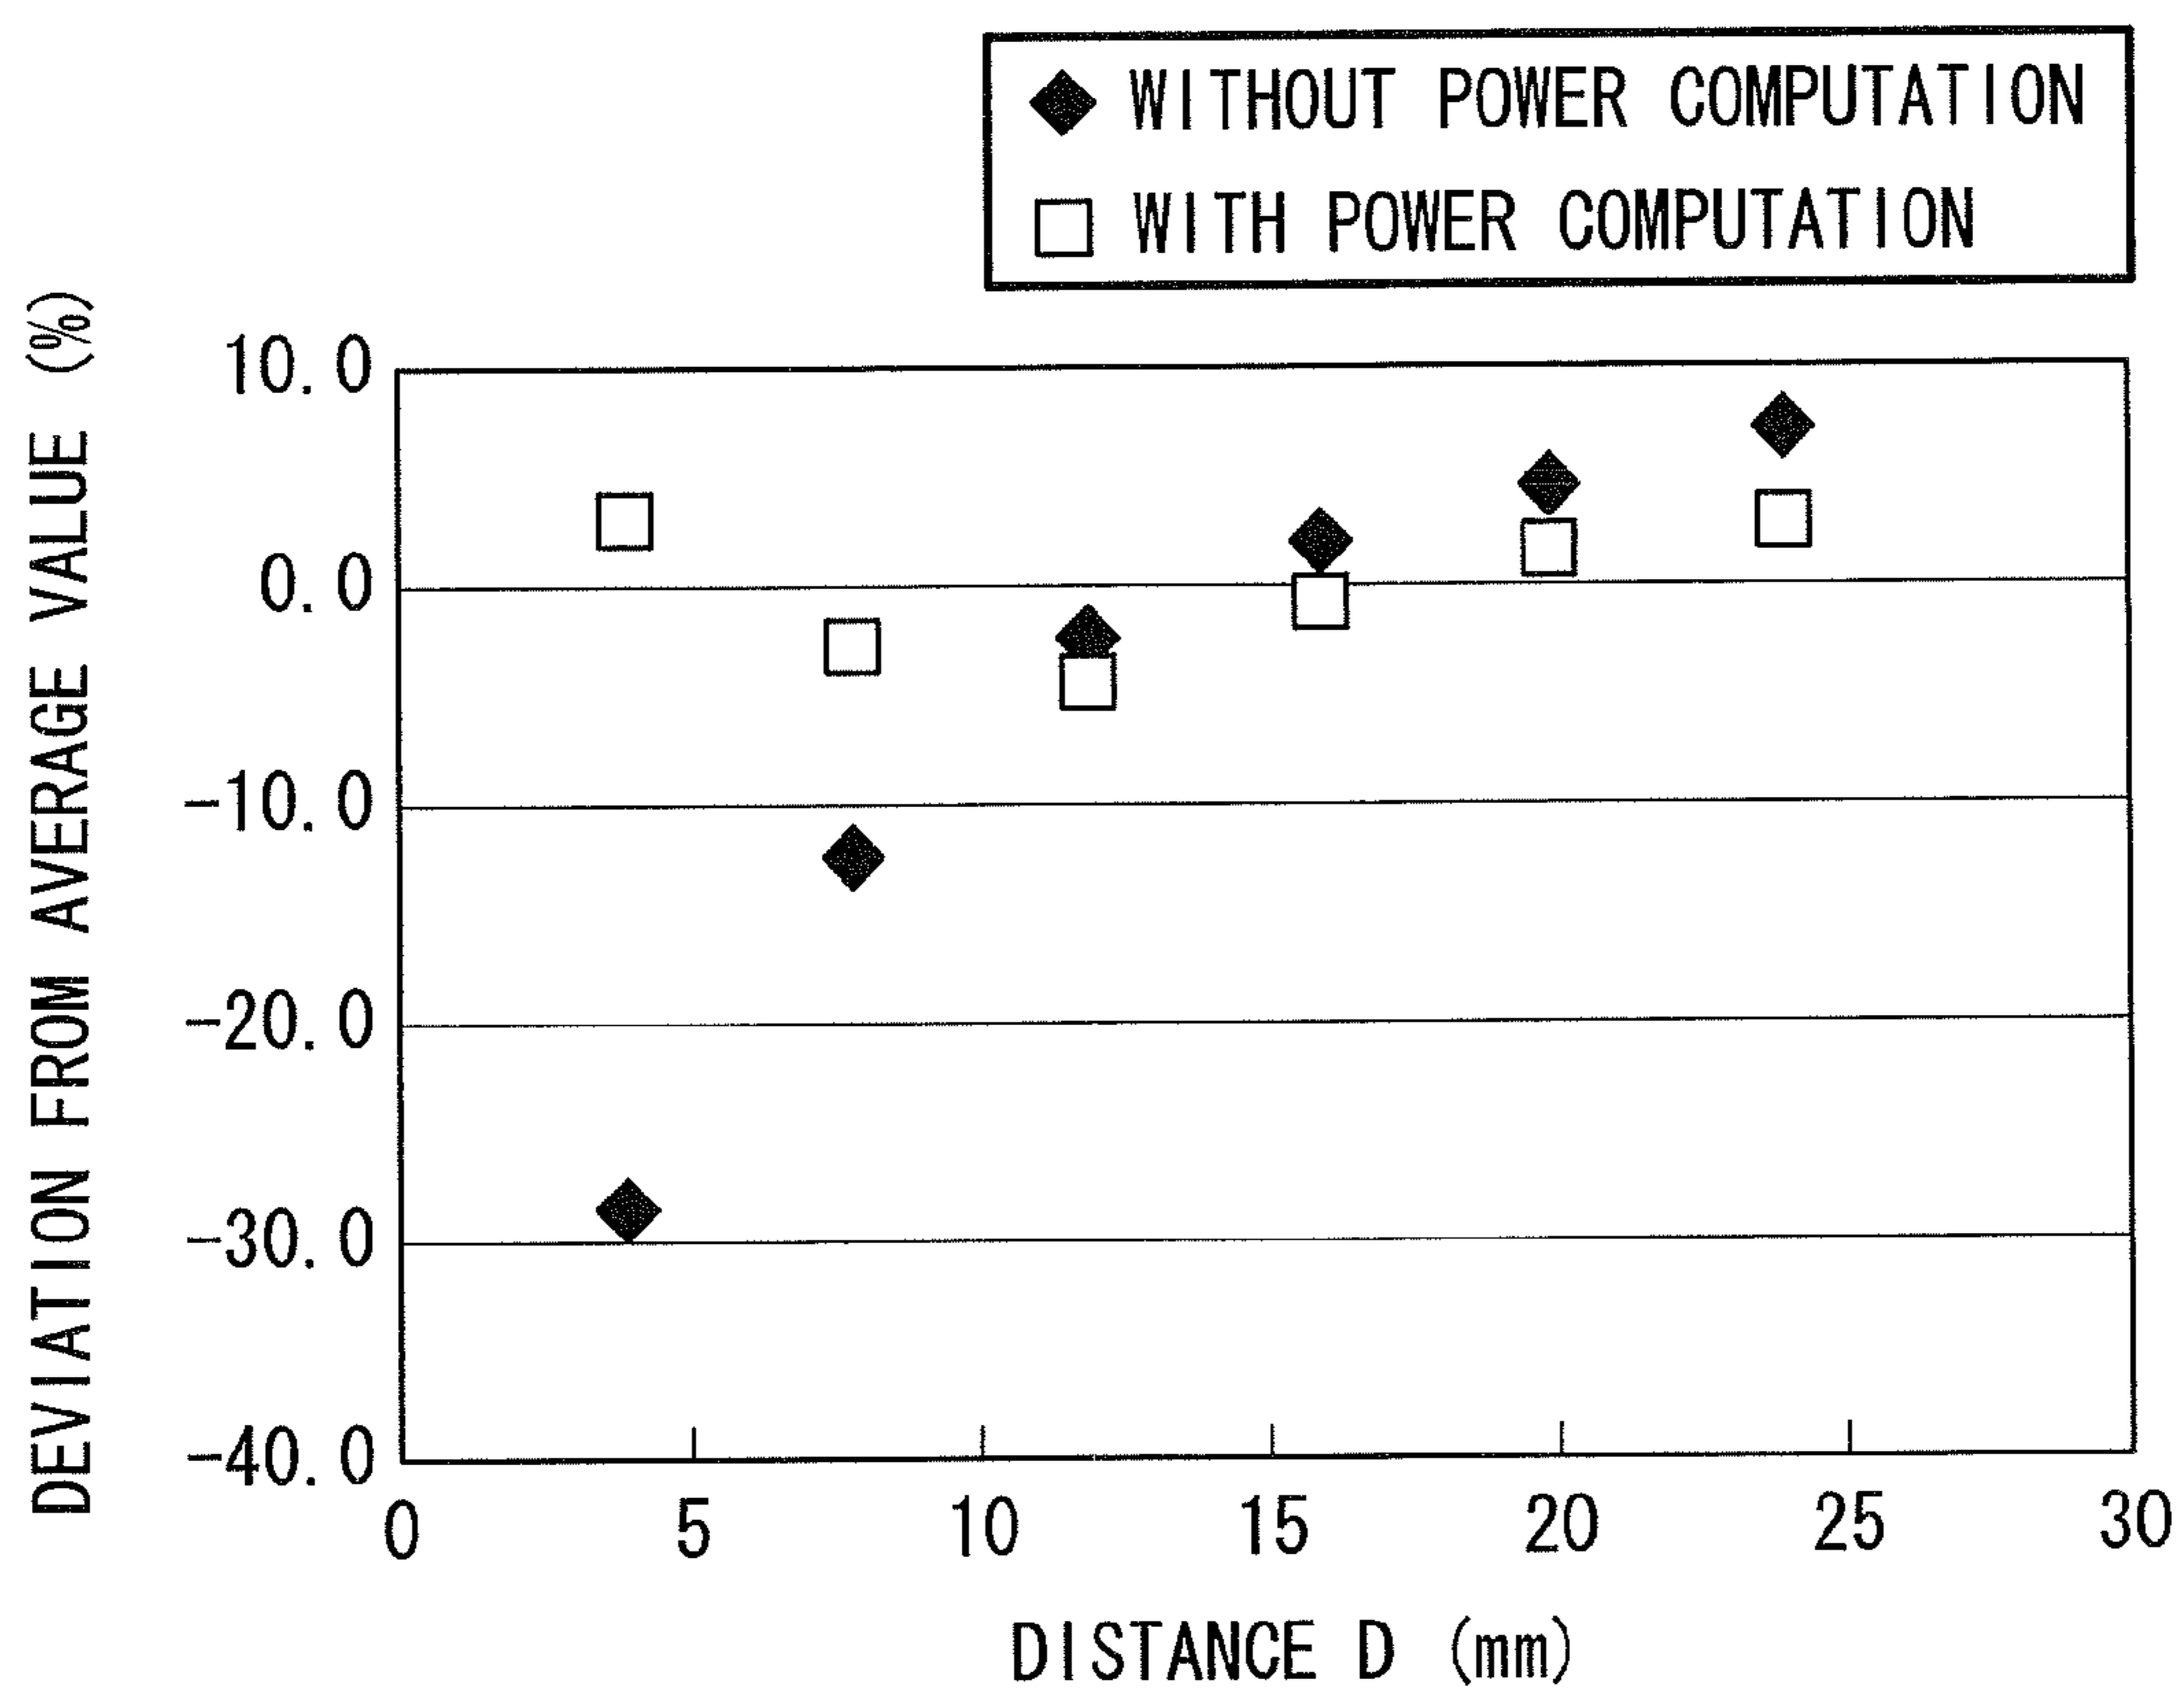


FIG. 10



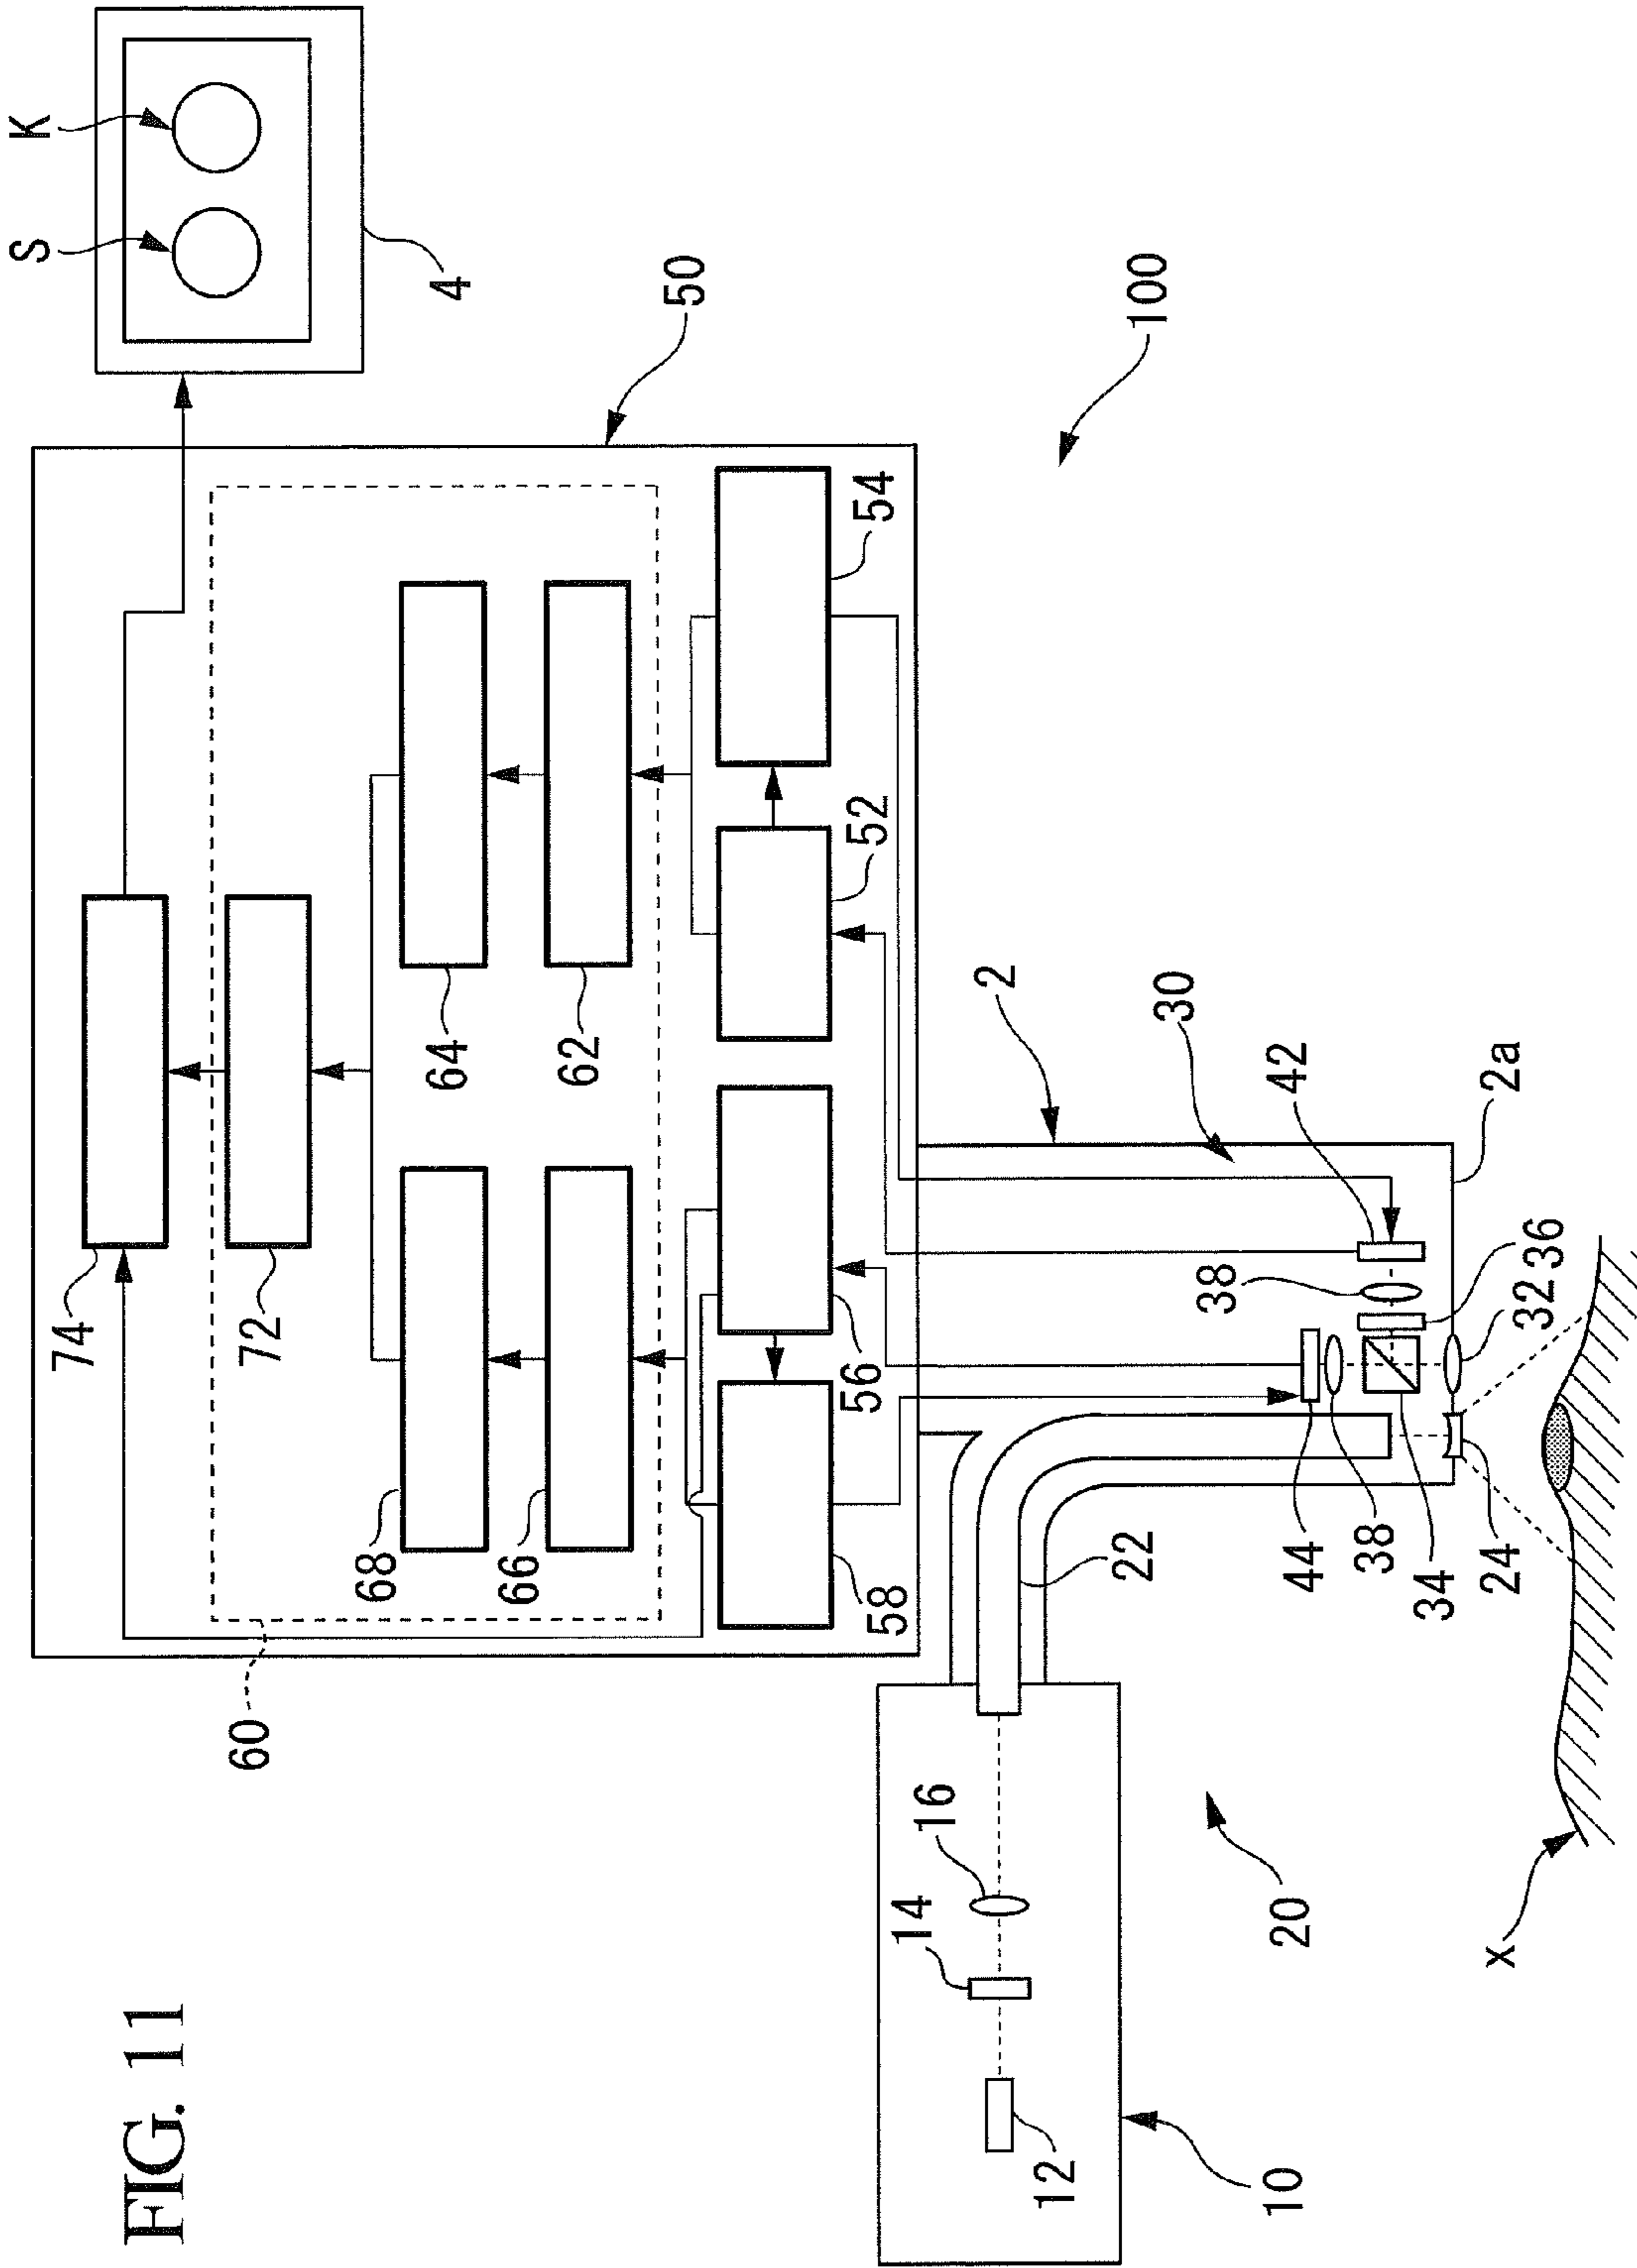


FIG. 11

FIG. 12

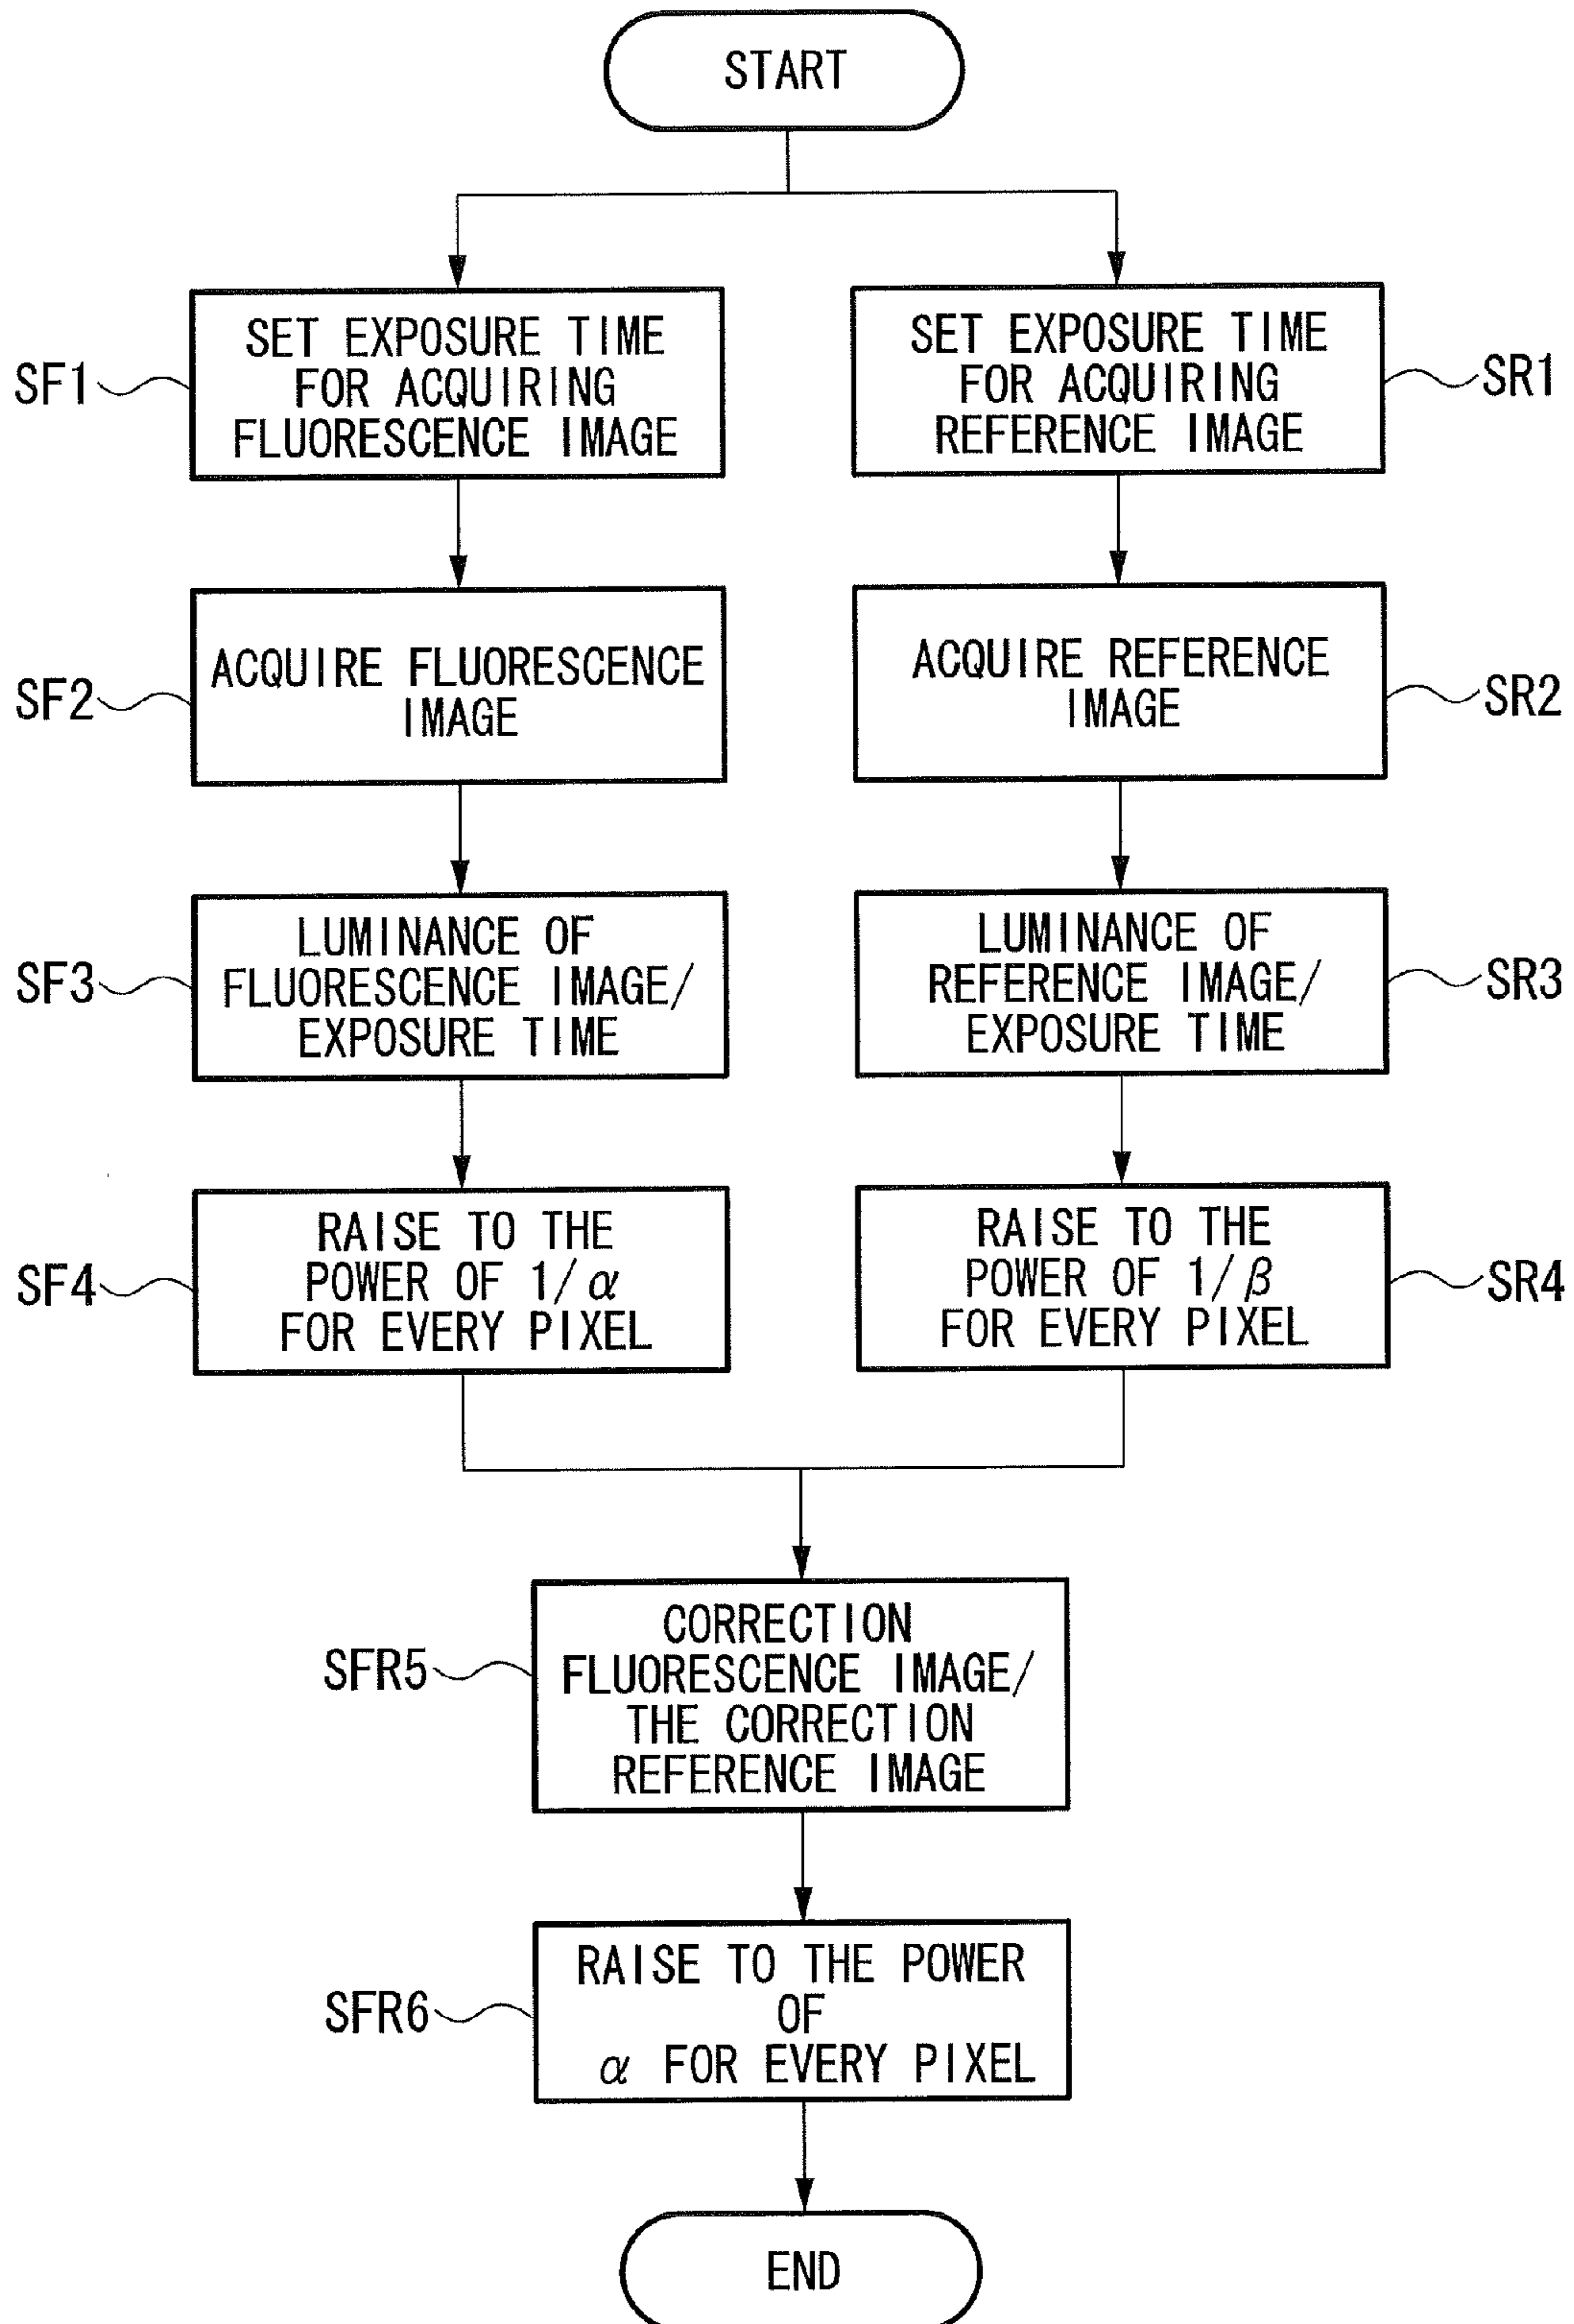


FIG. 13

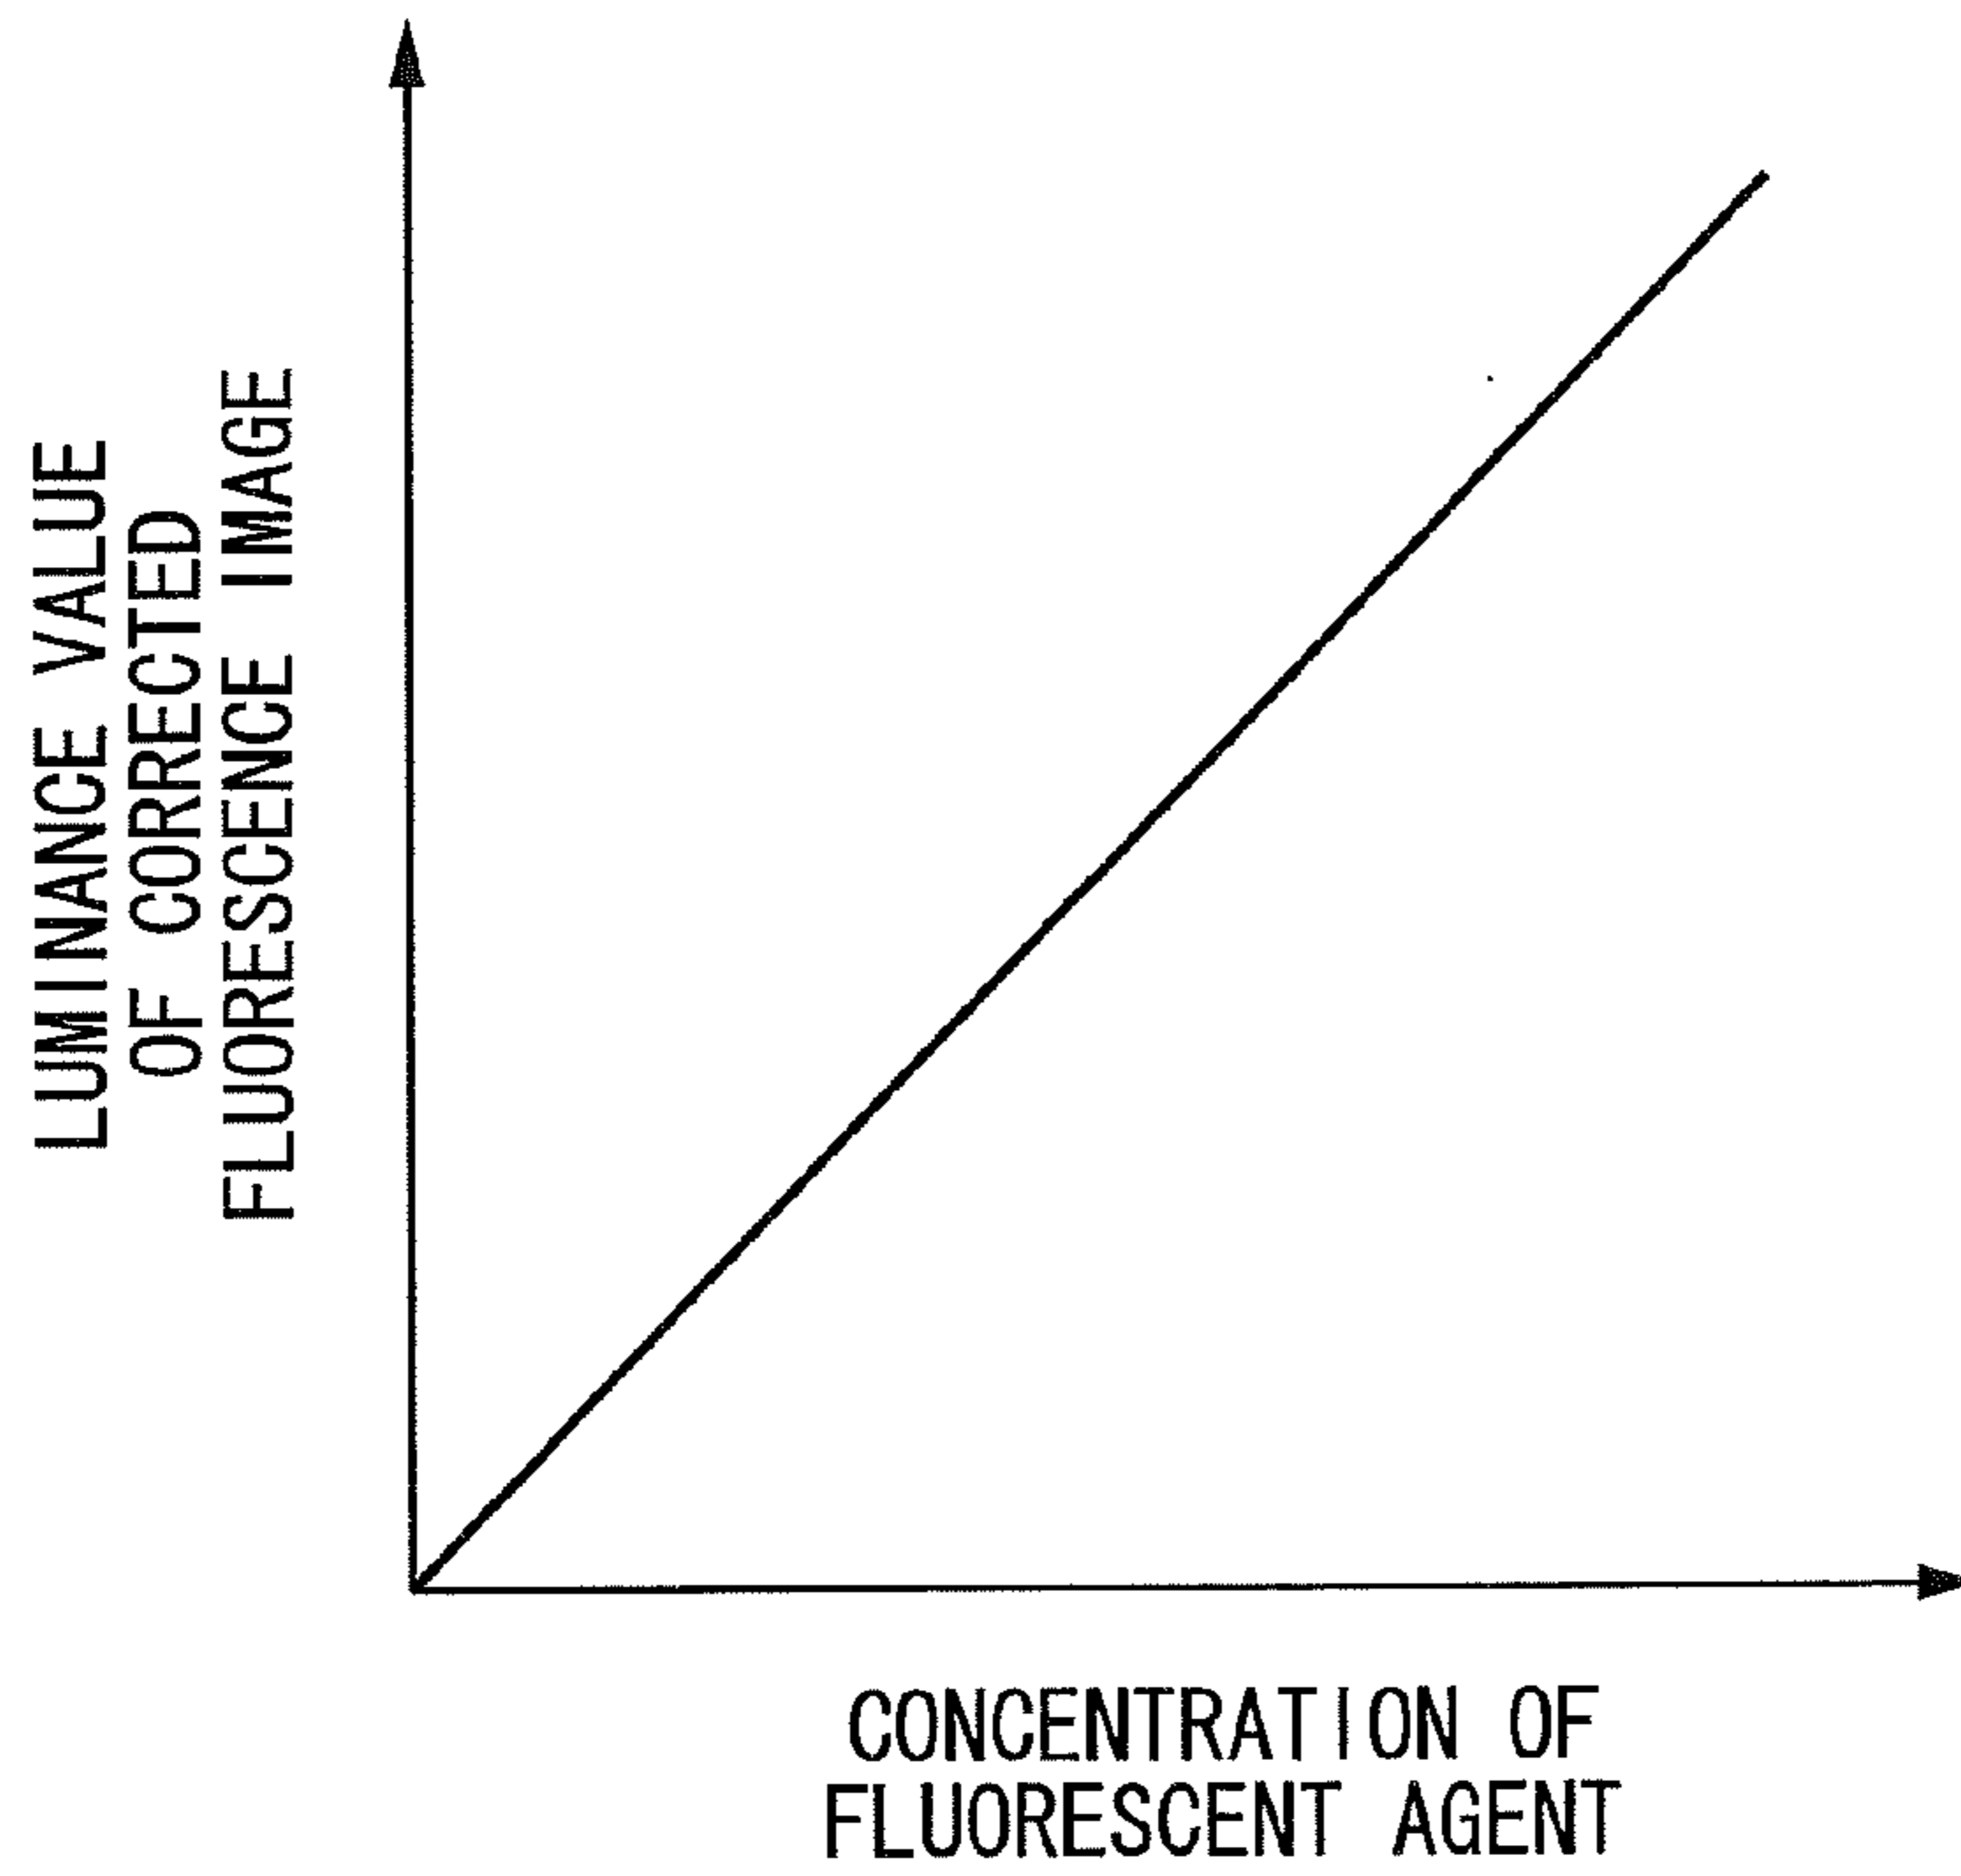


FIG. 14

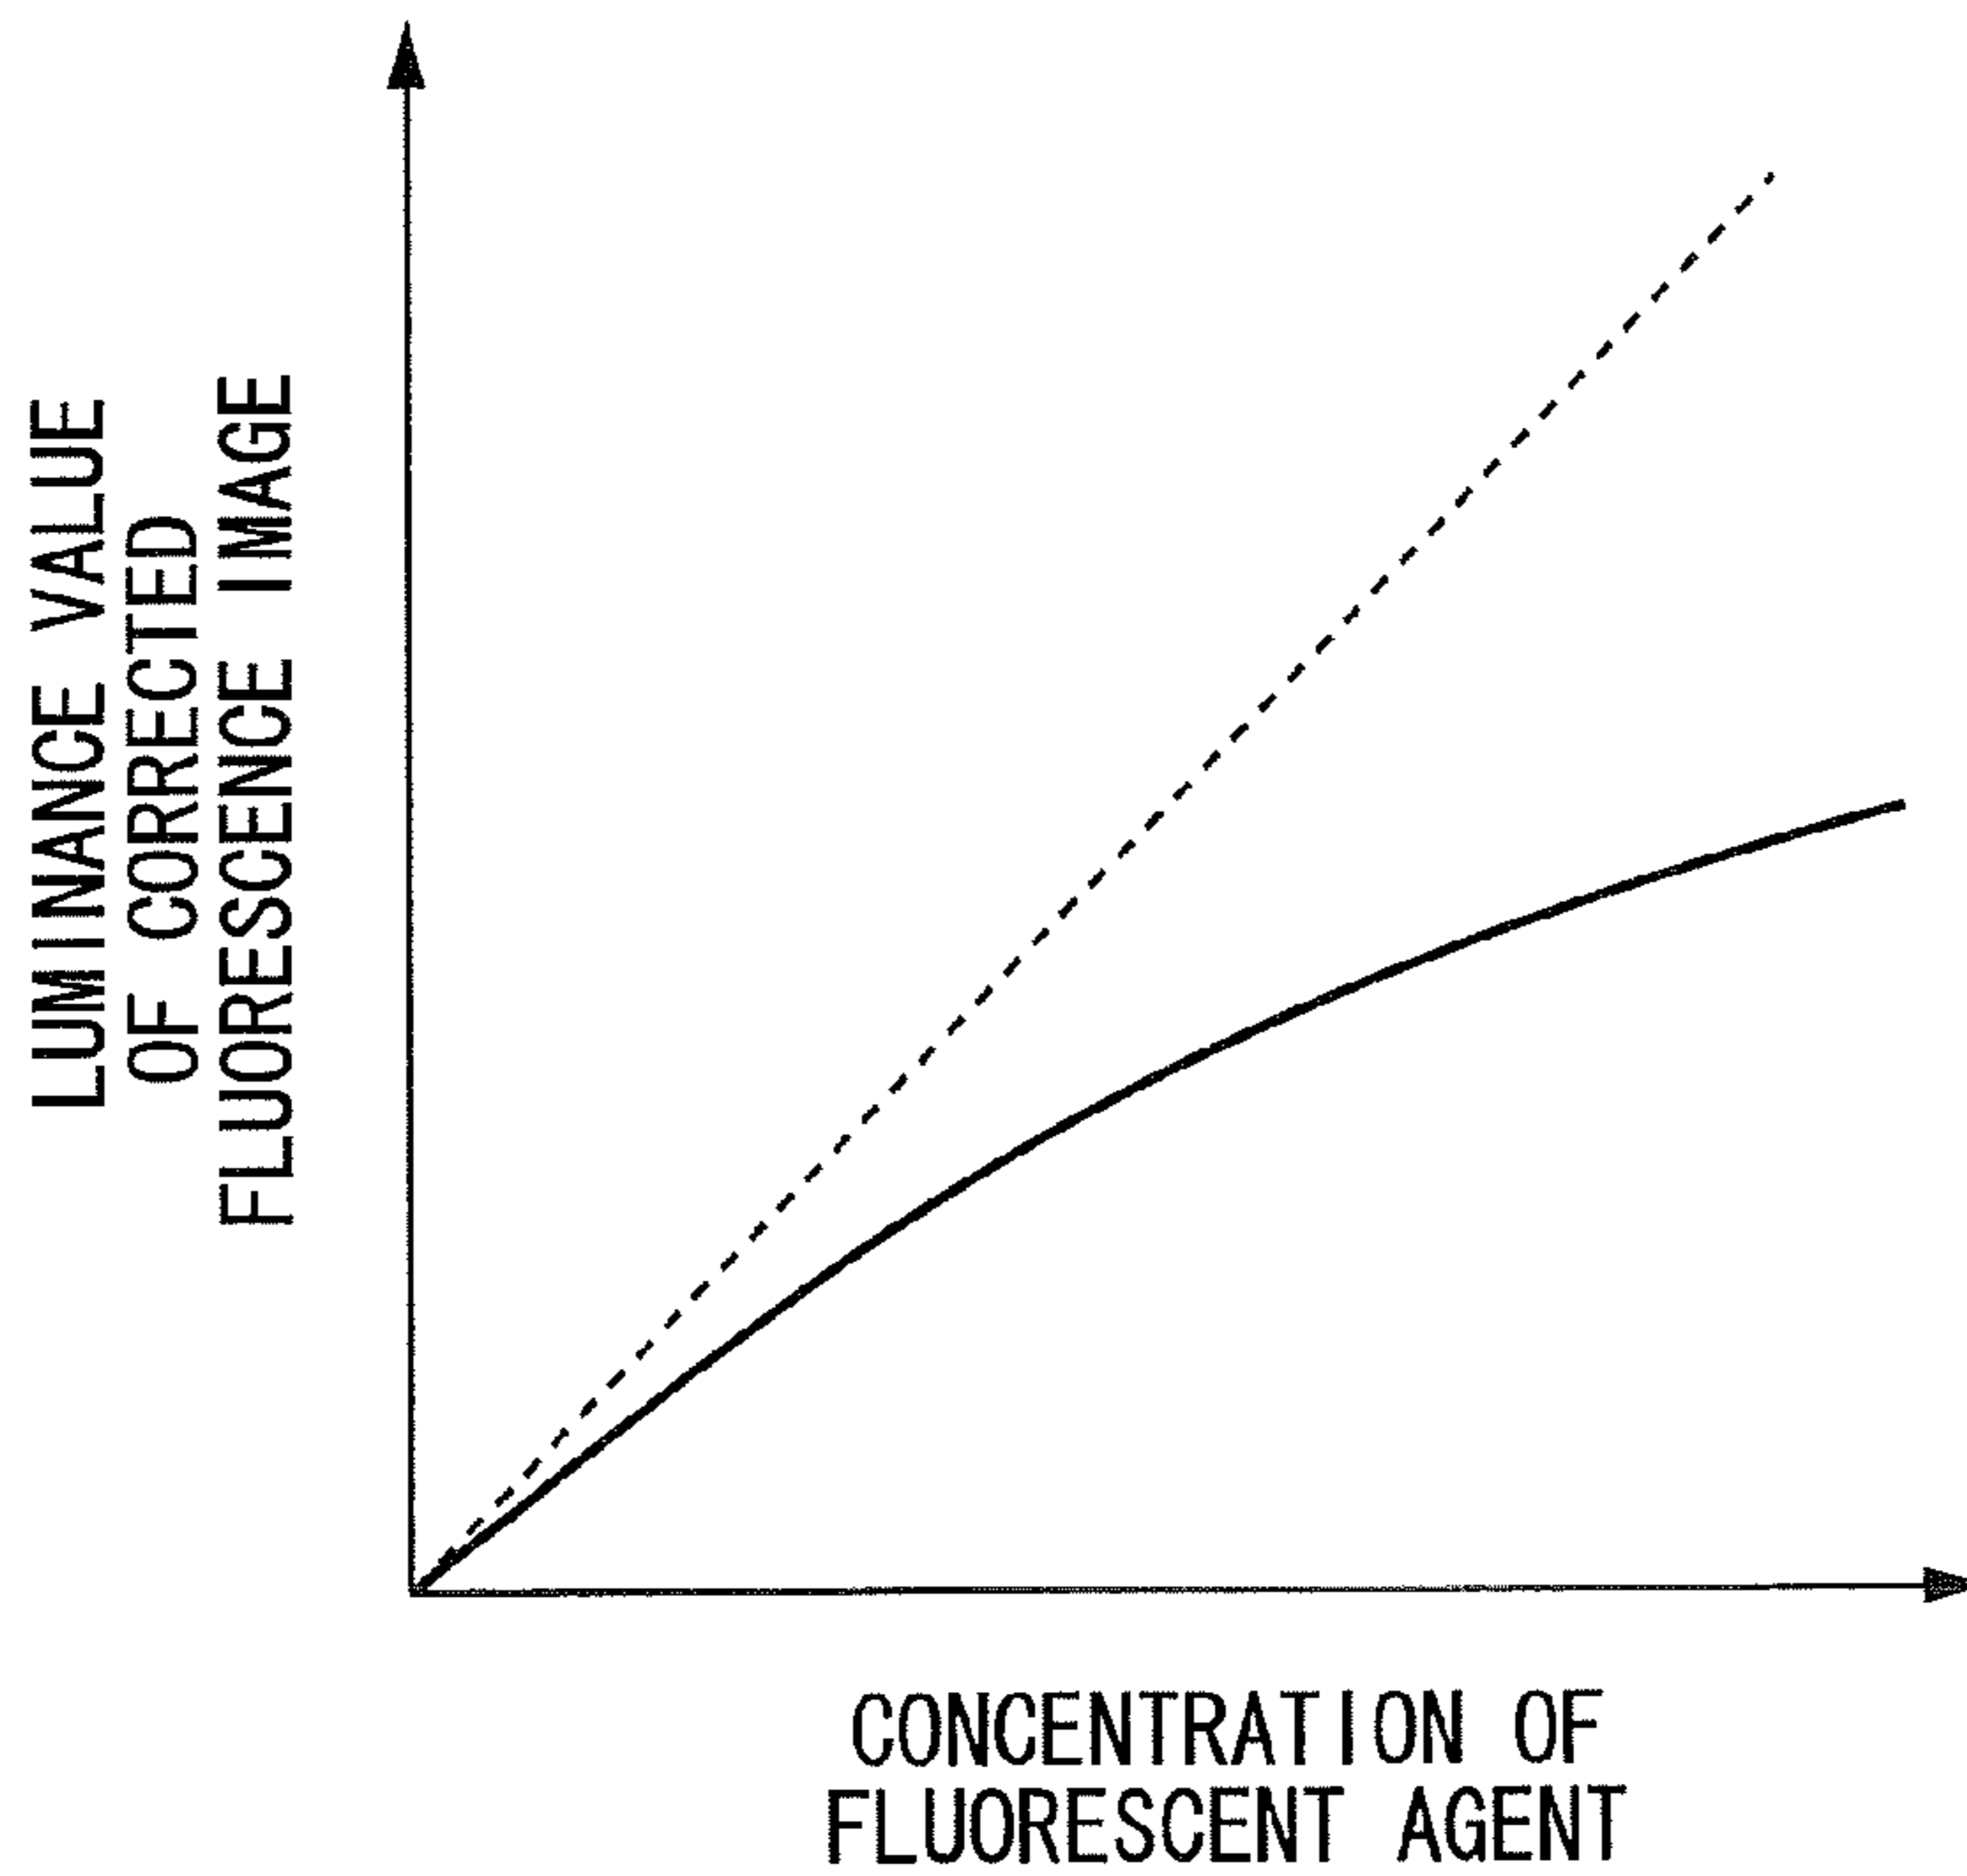


FIG. 15

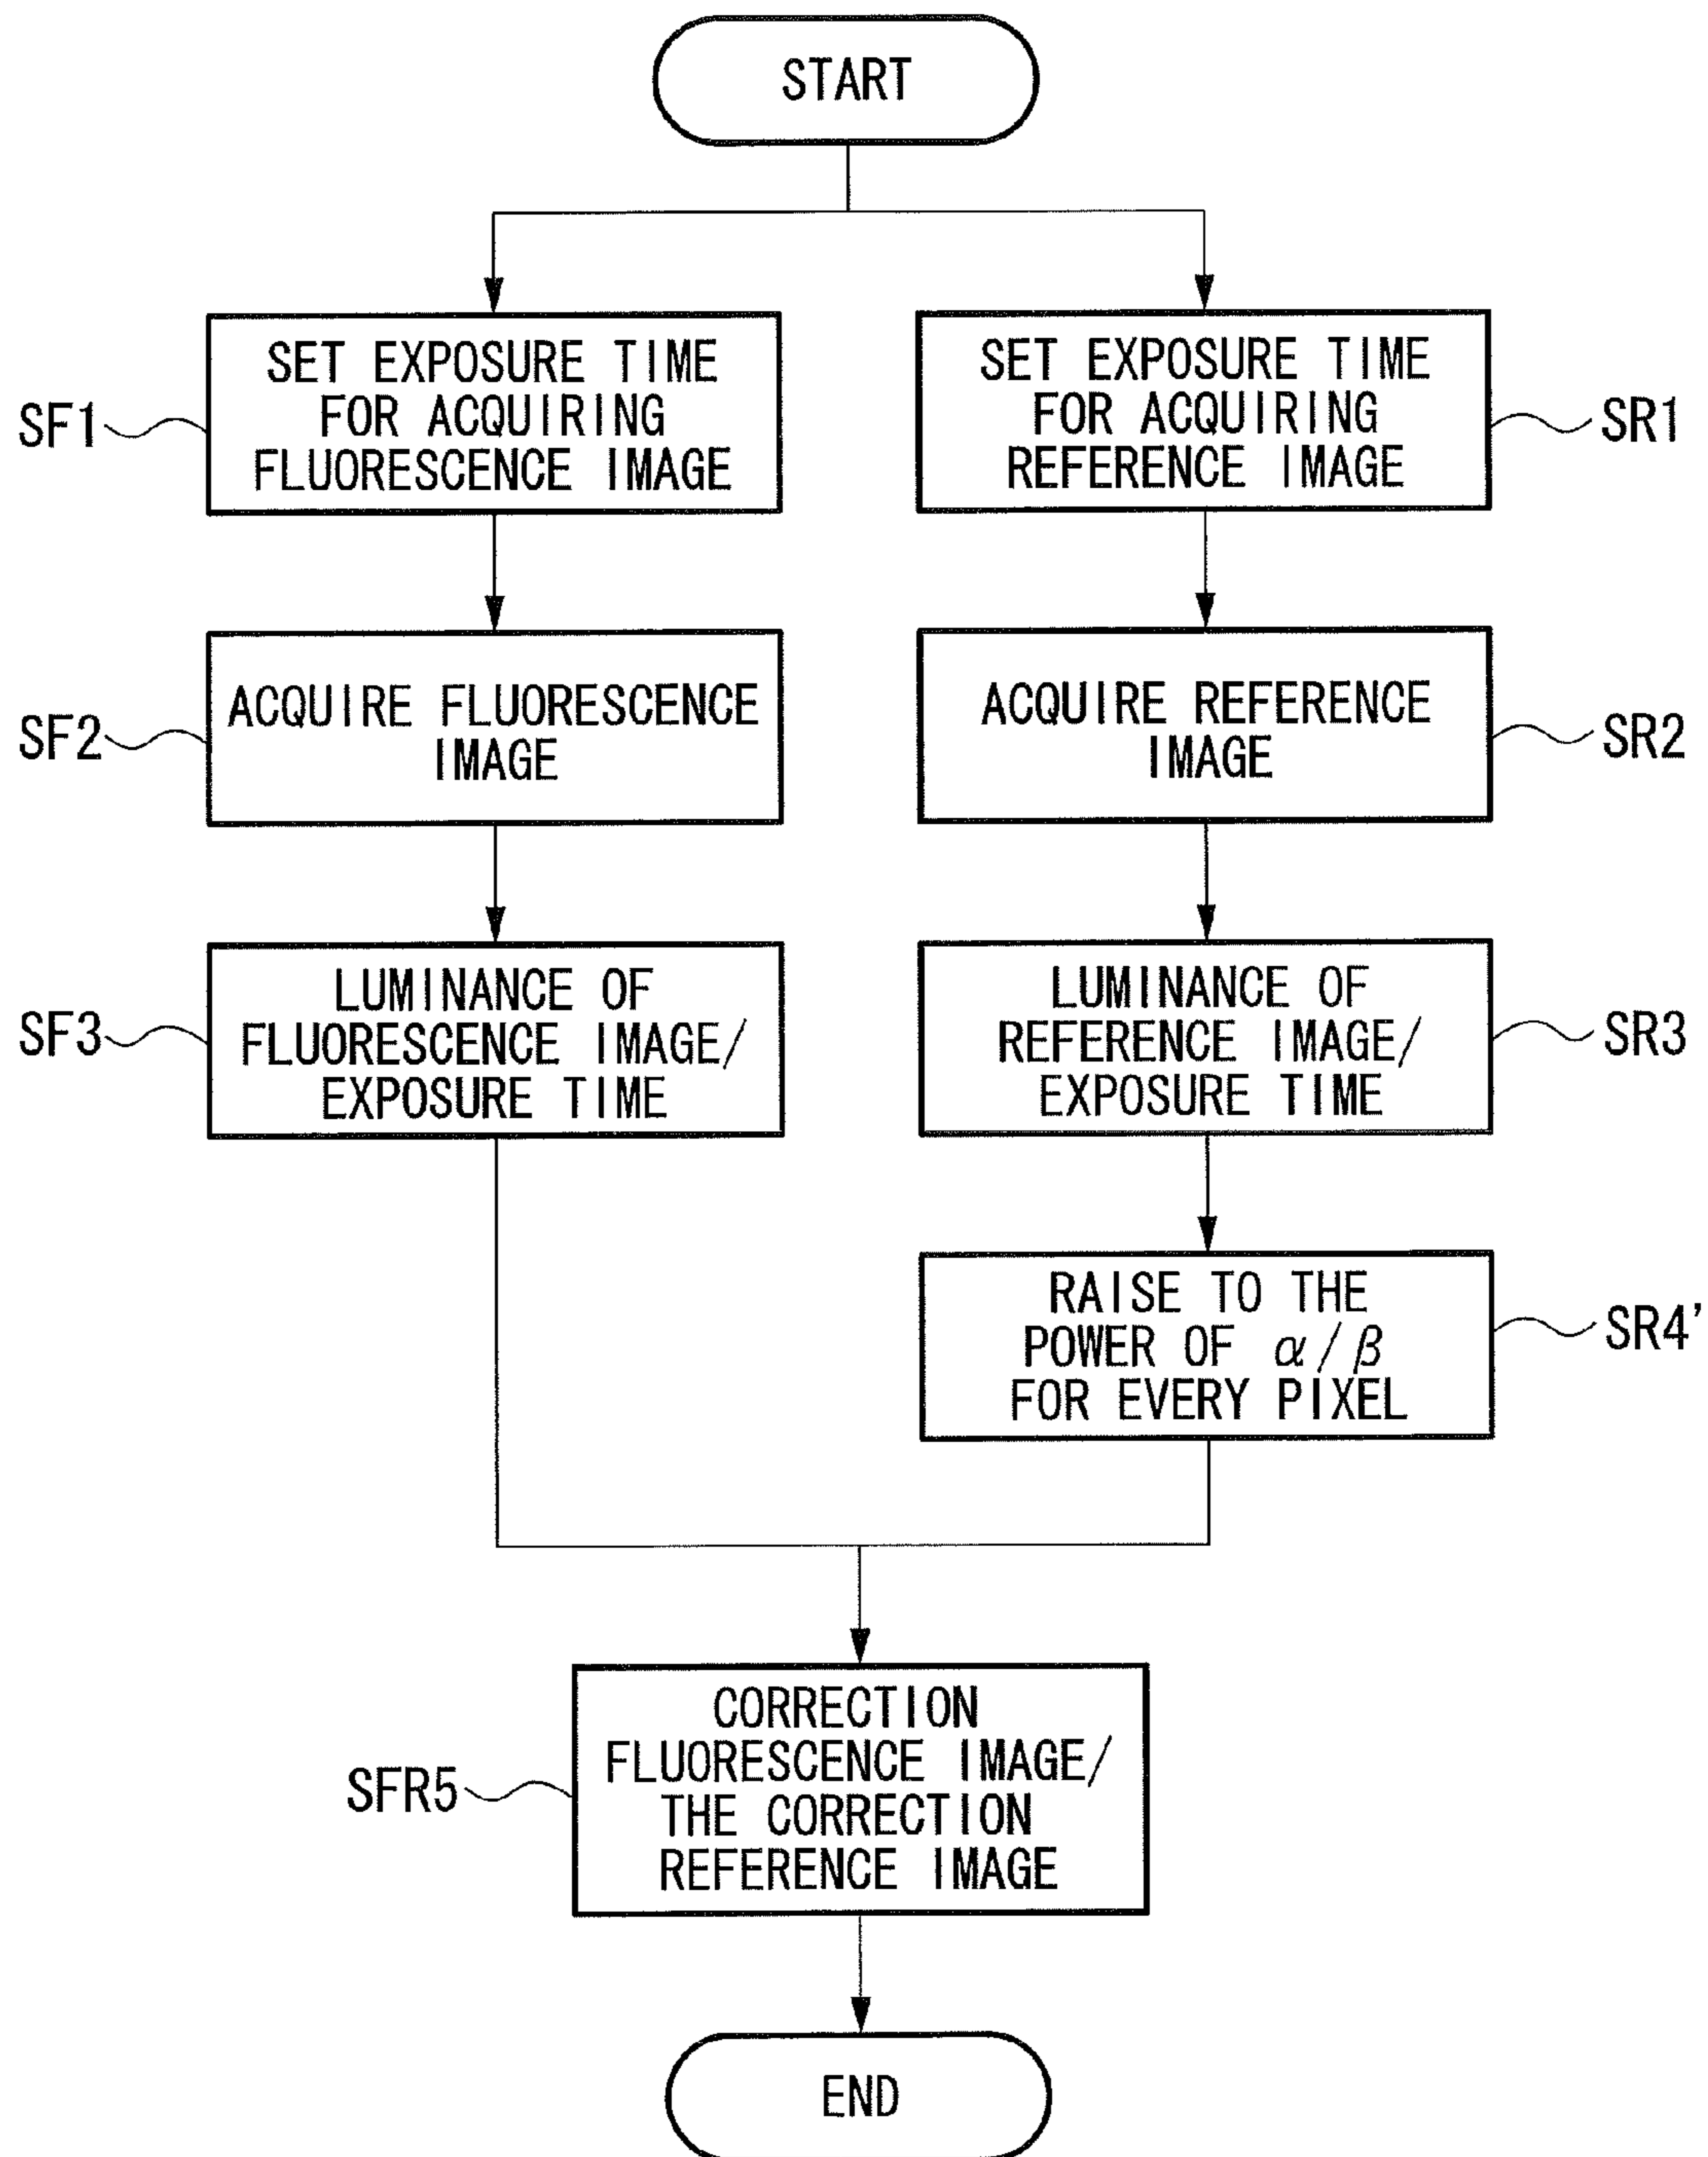


FIG. 16

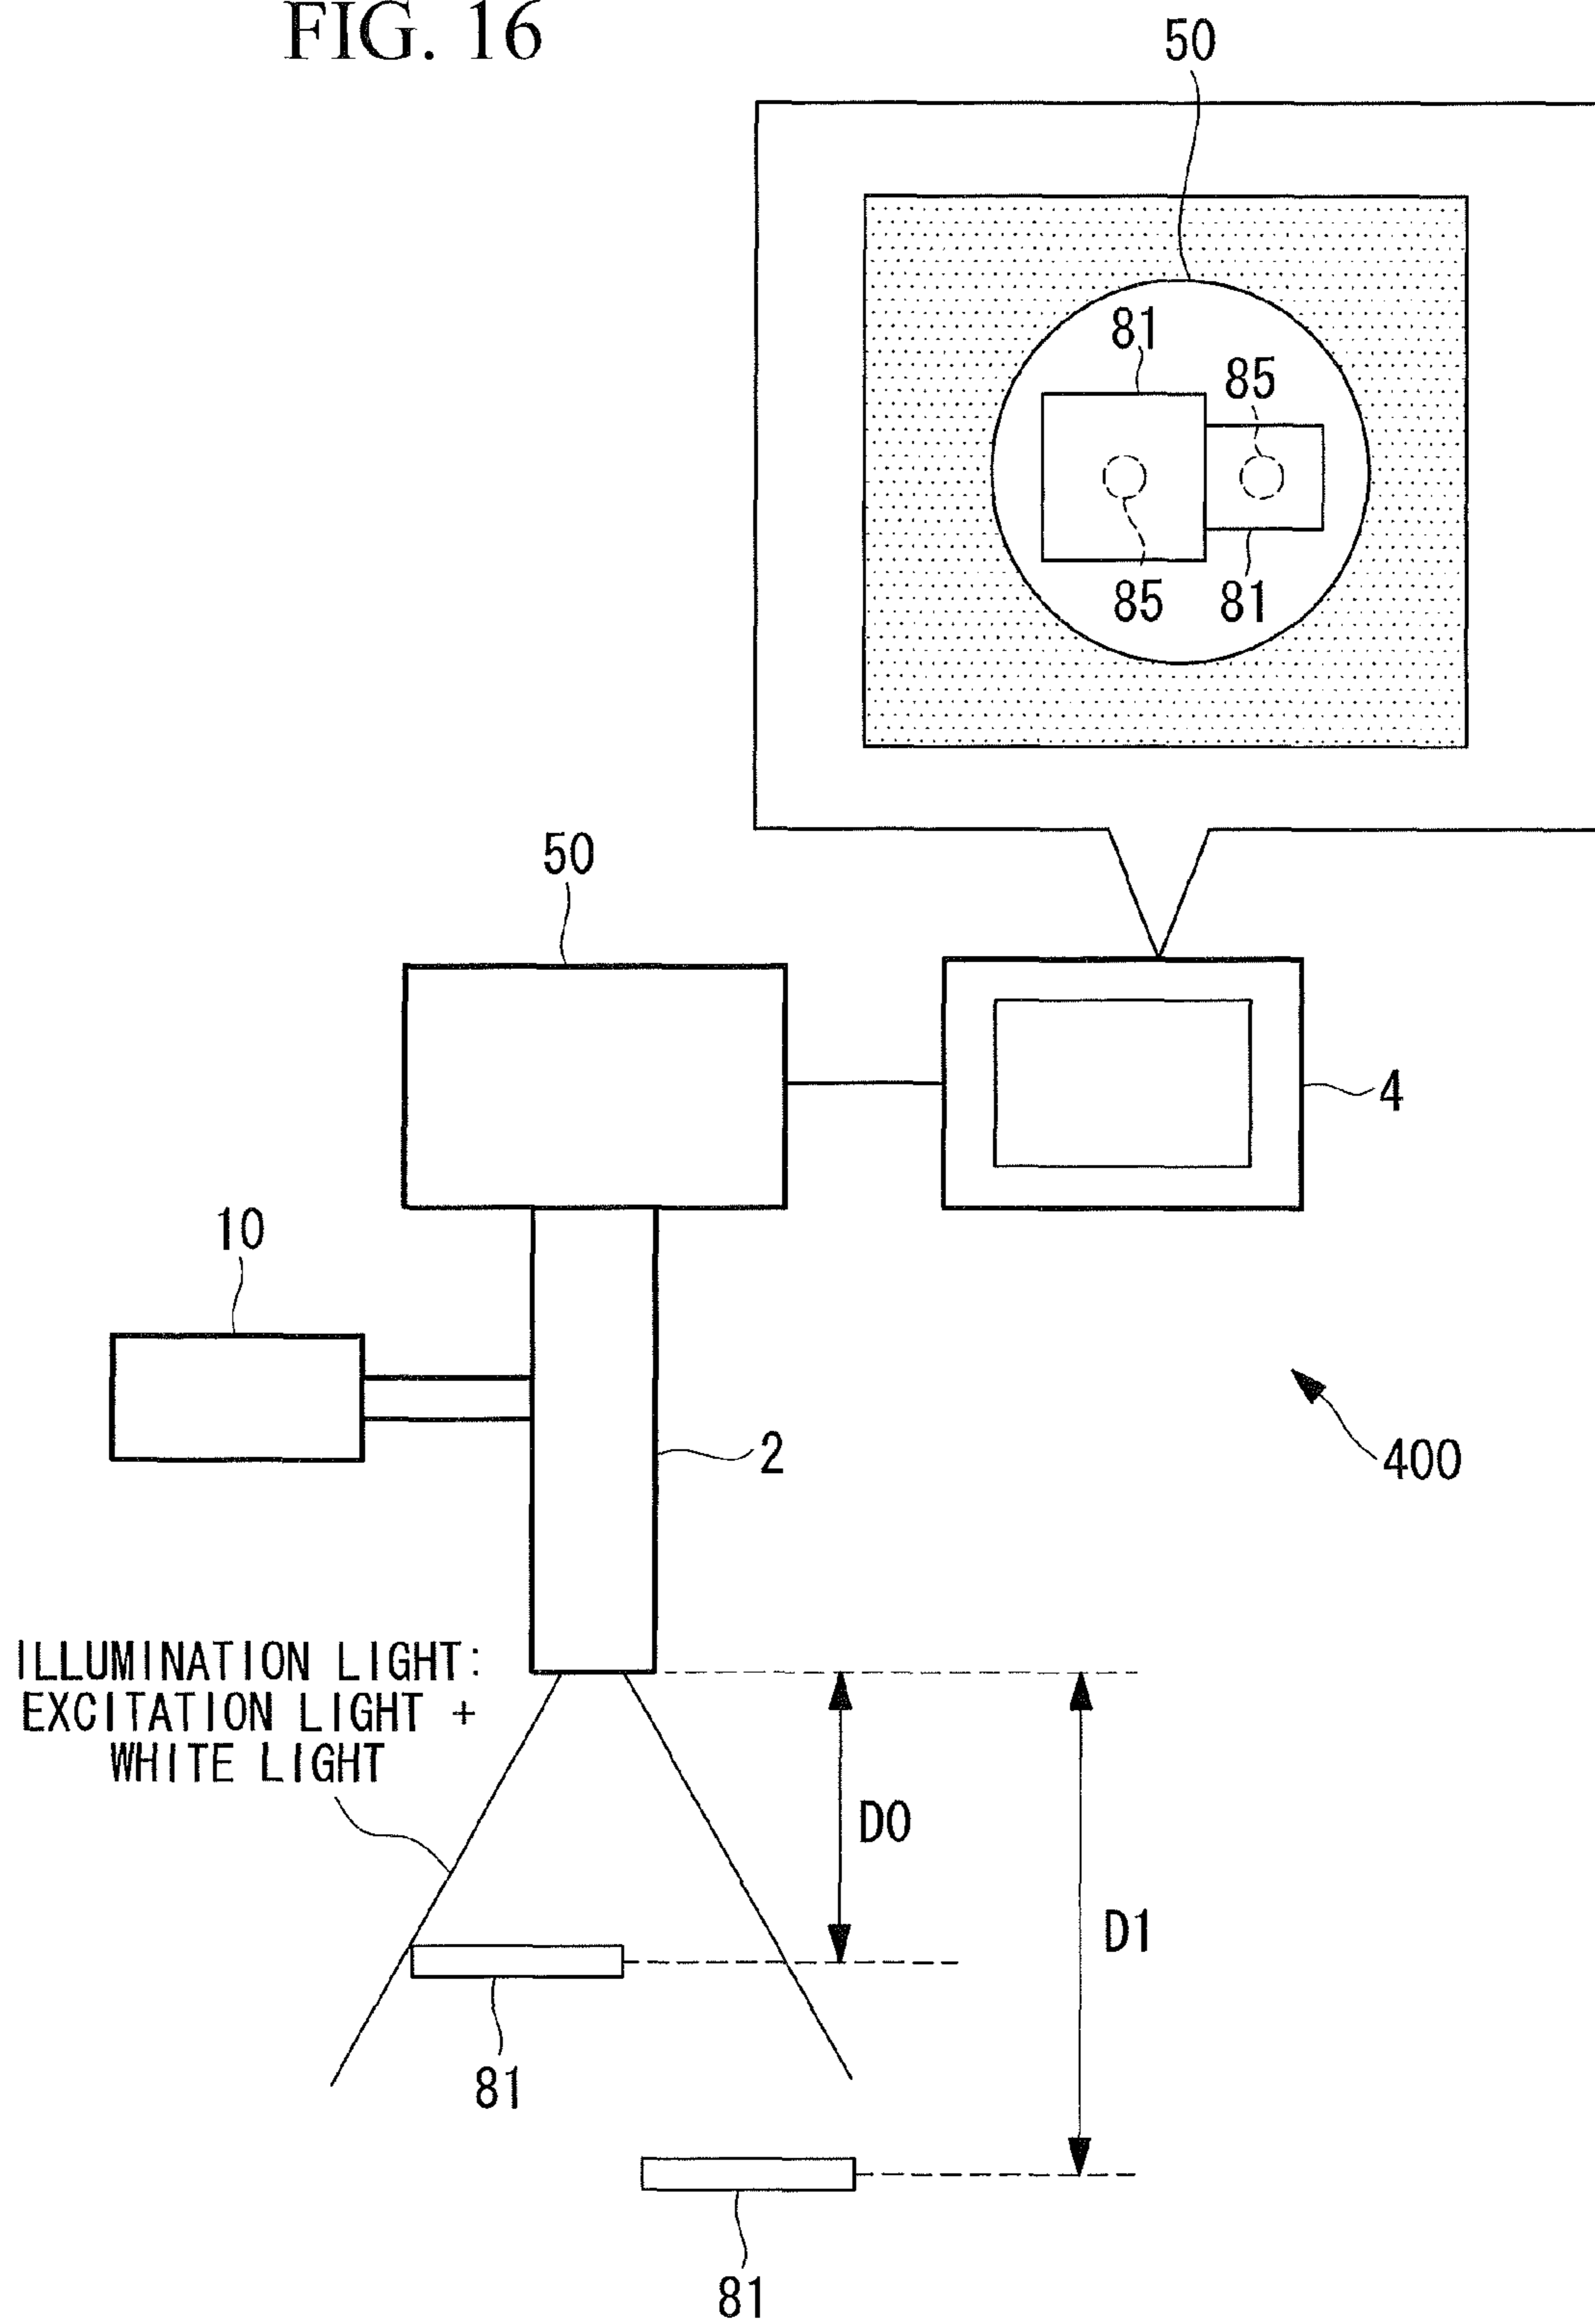


FIG. 17A

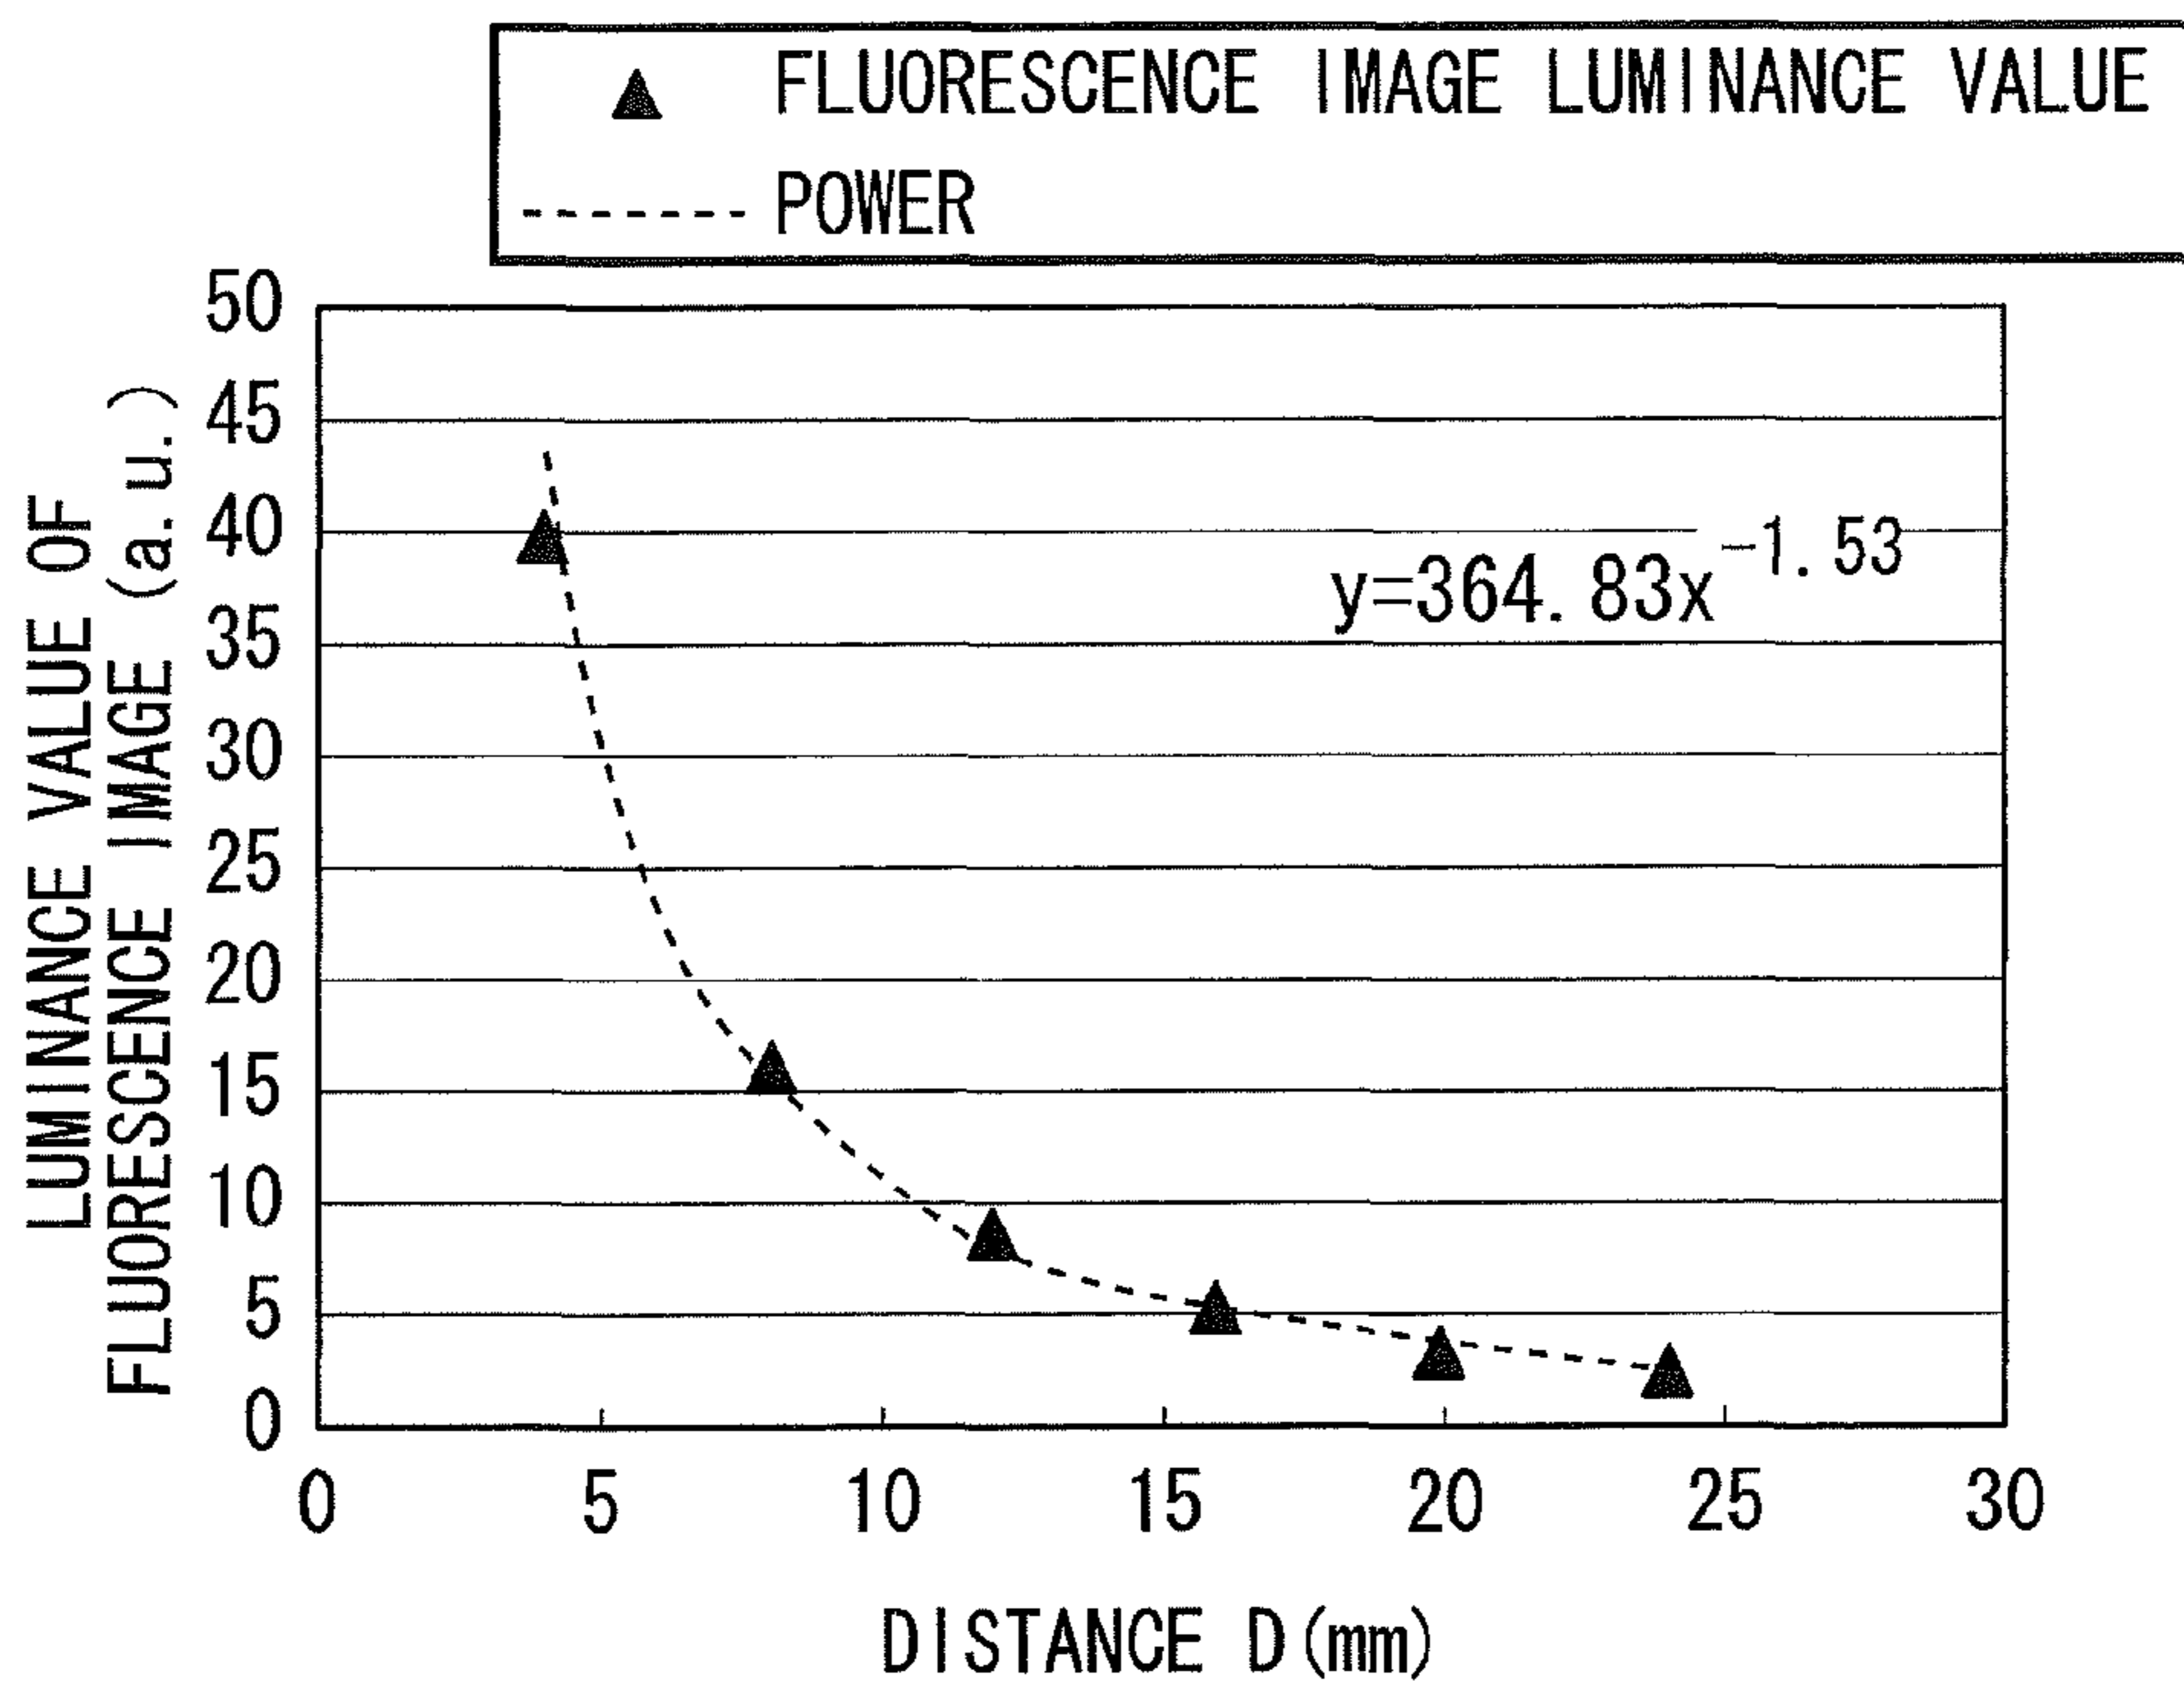


FIG. 17B

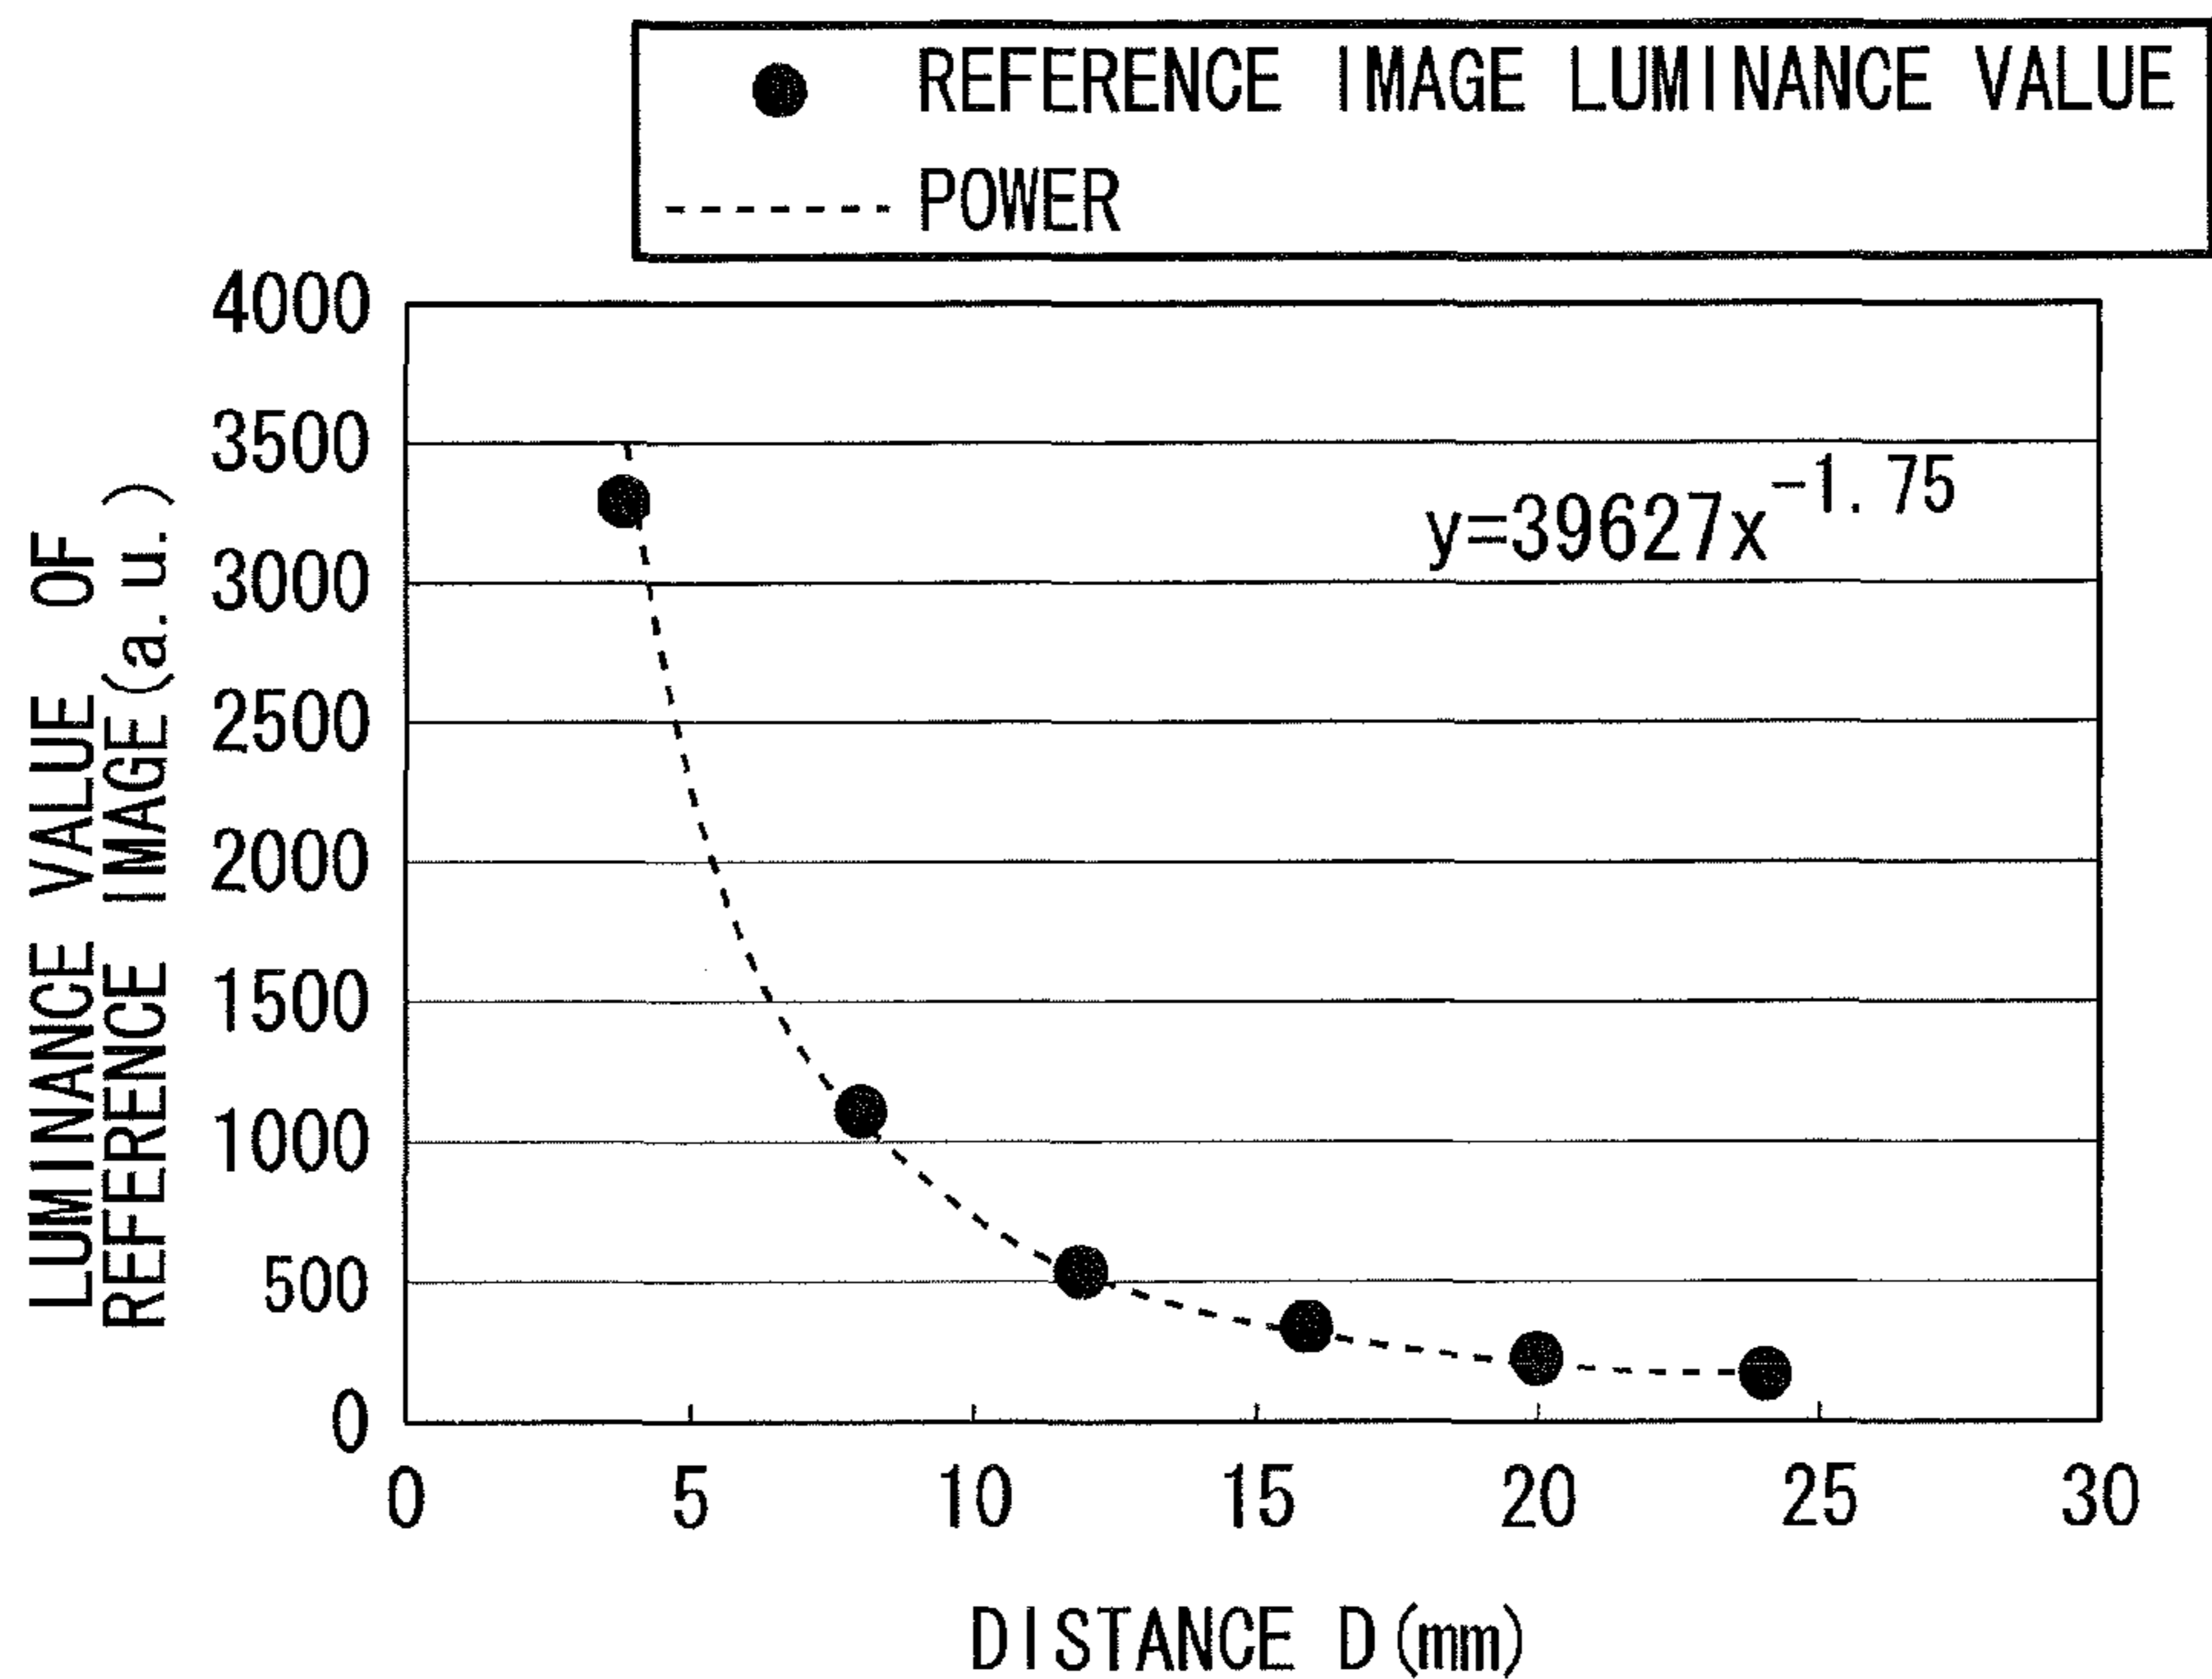


FIG. 18

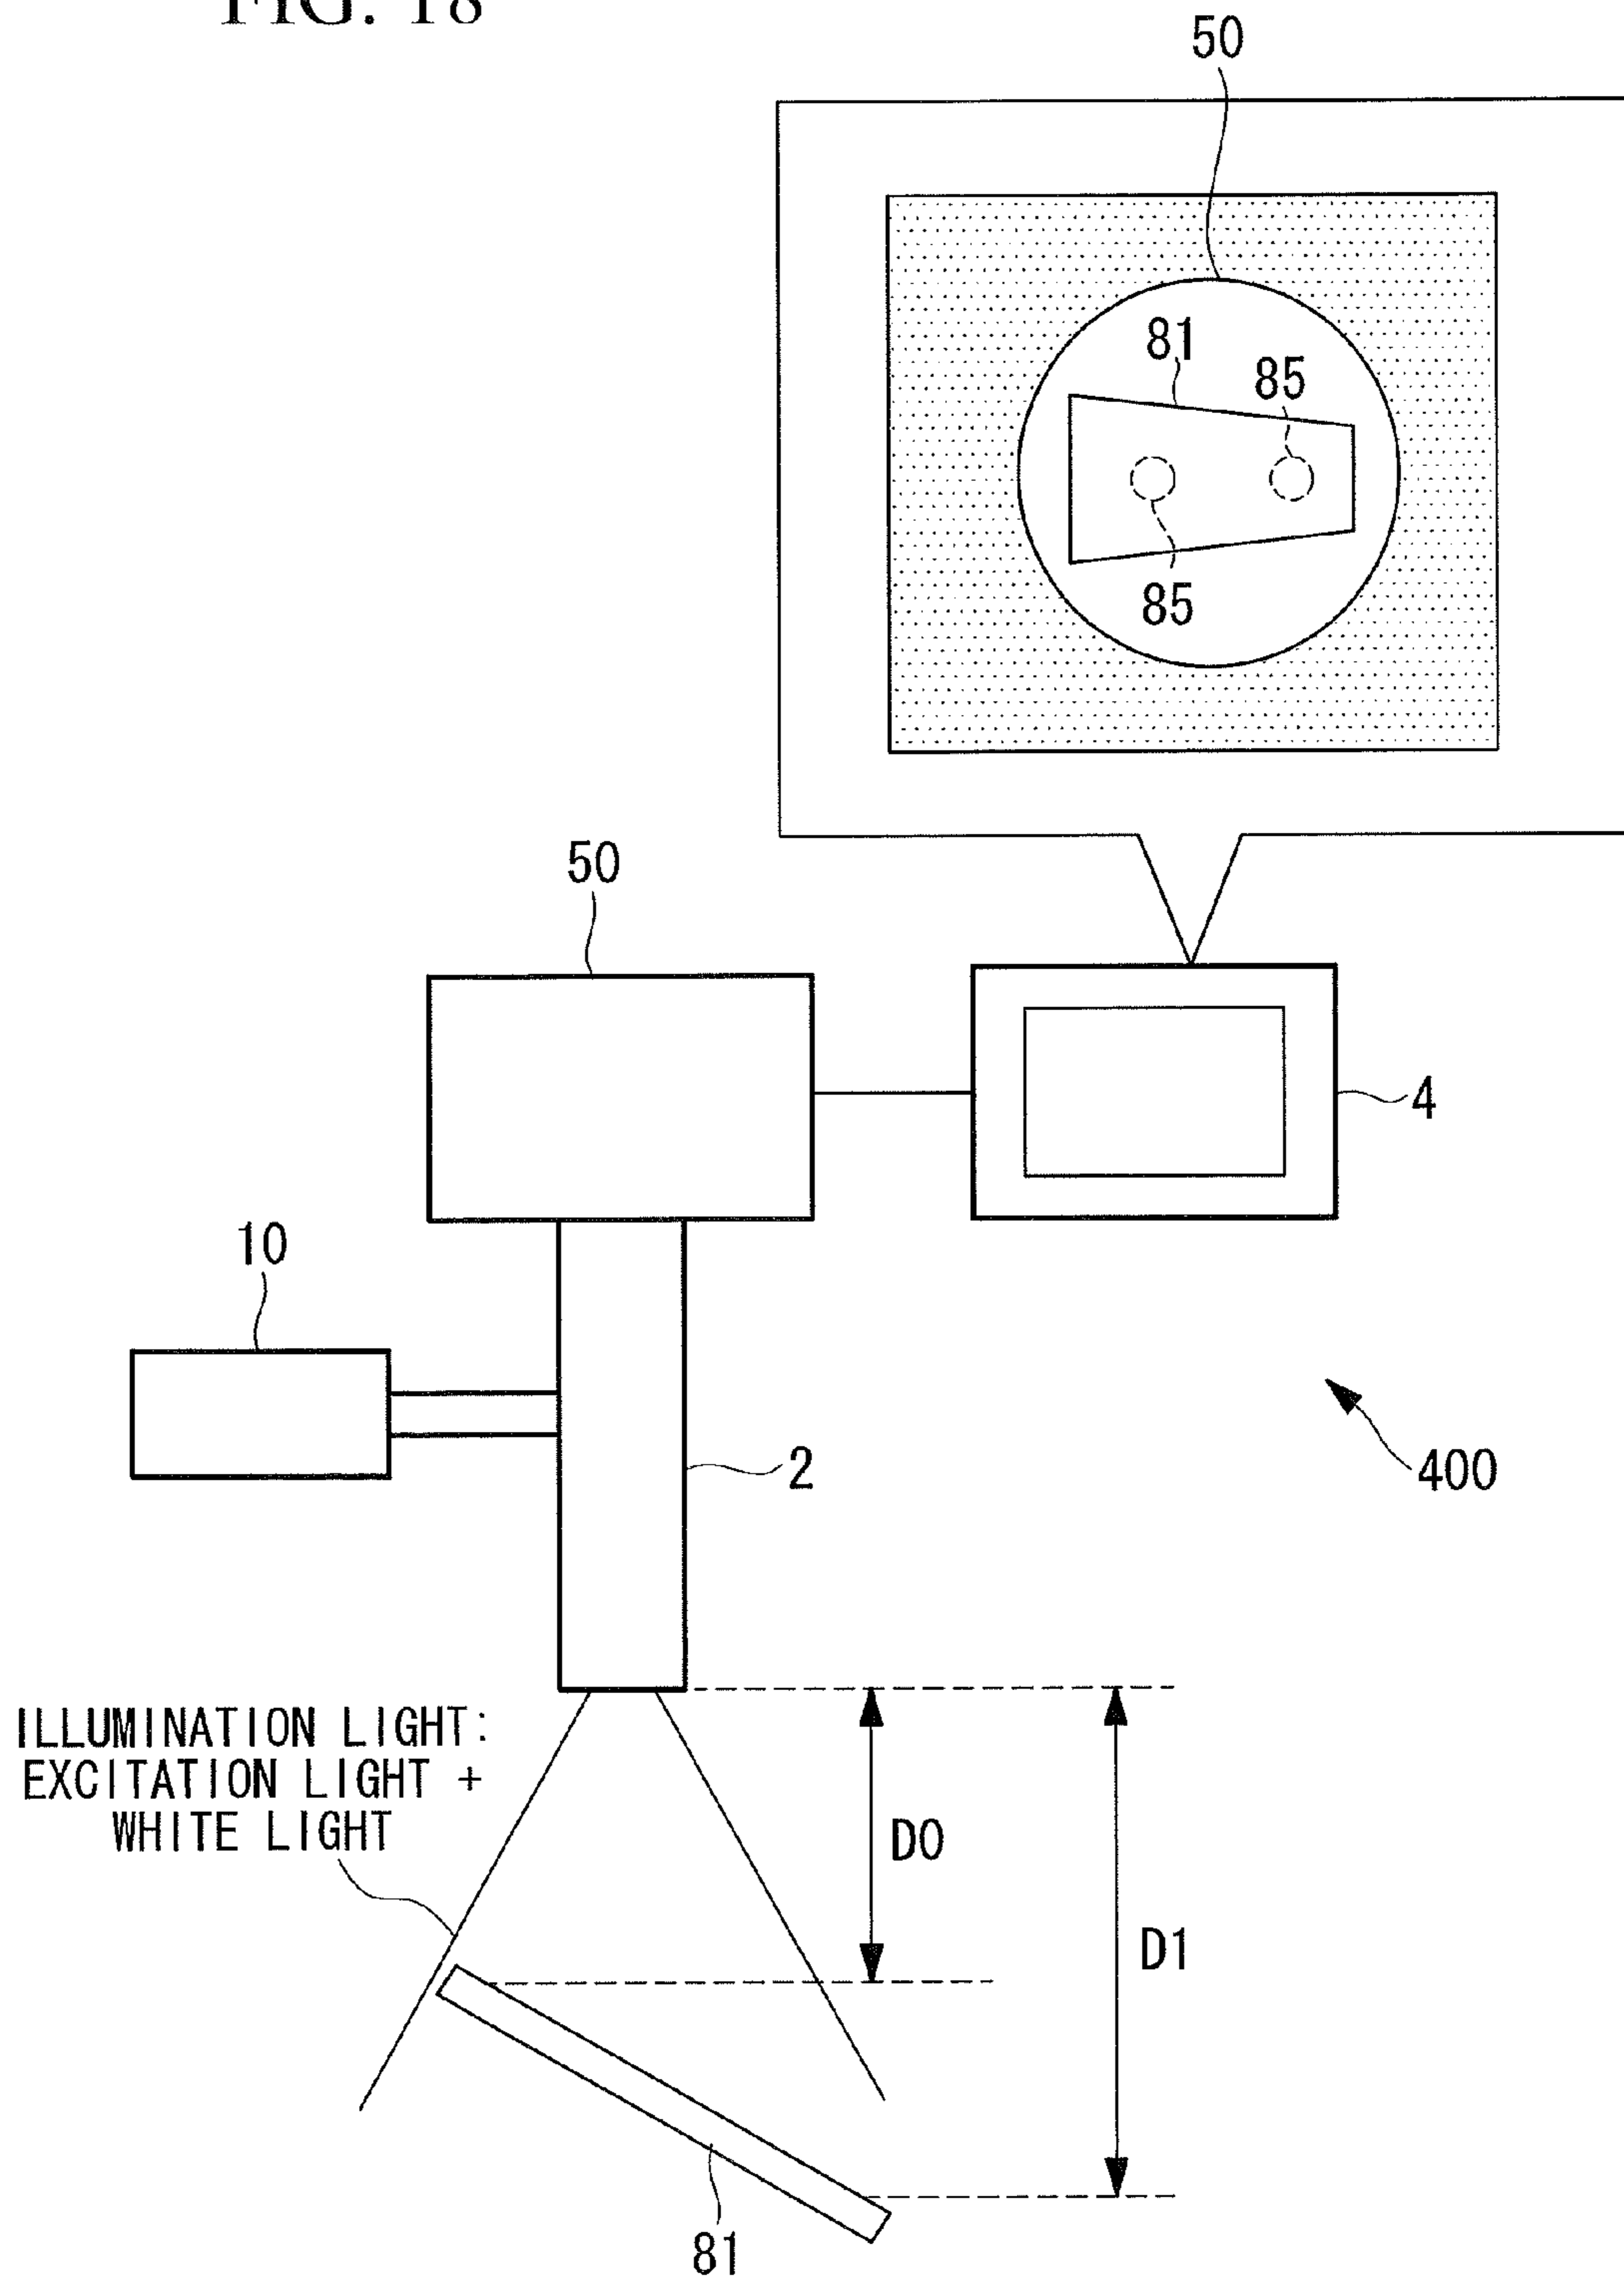


FIG. 19

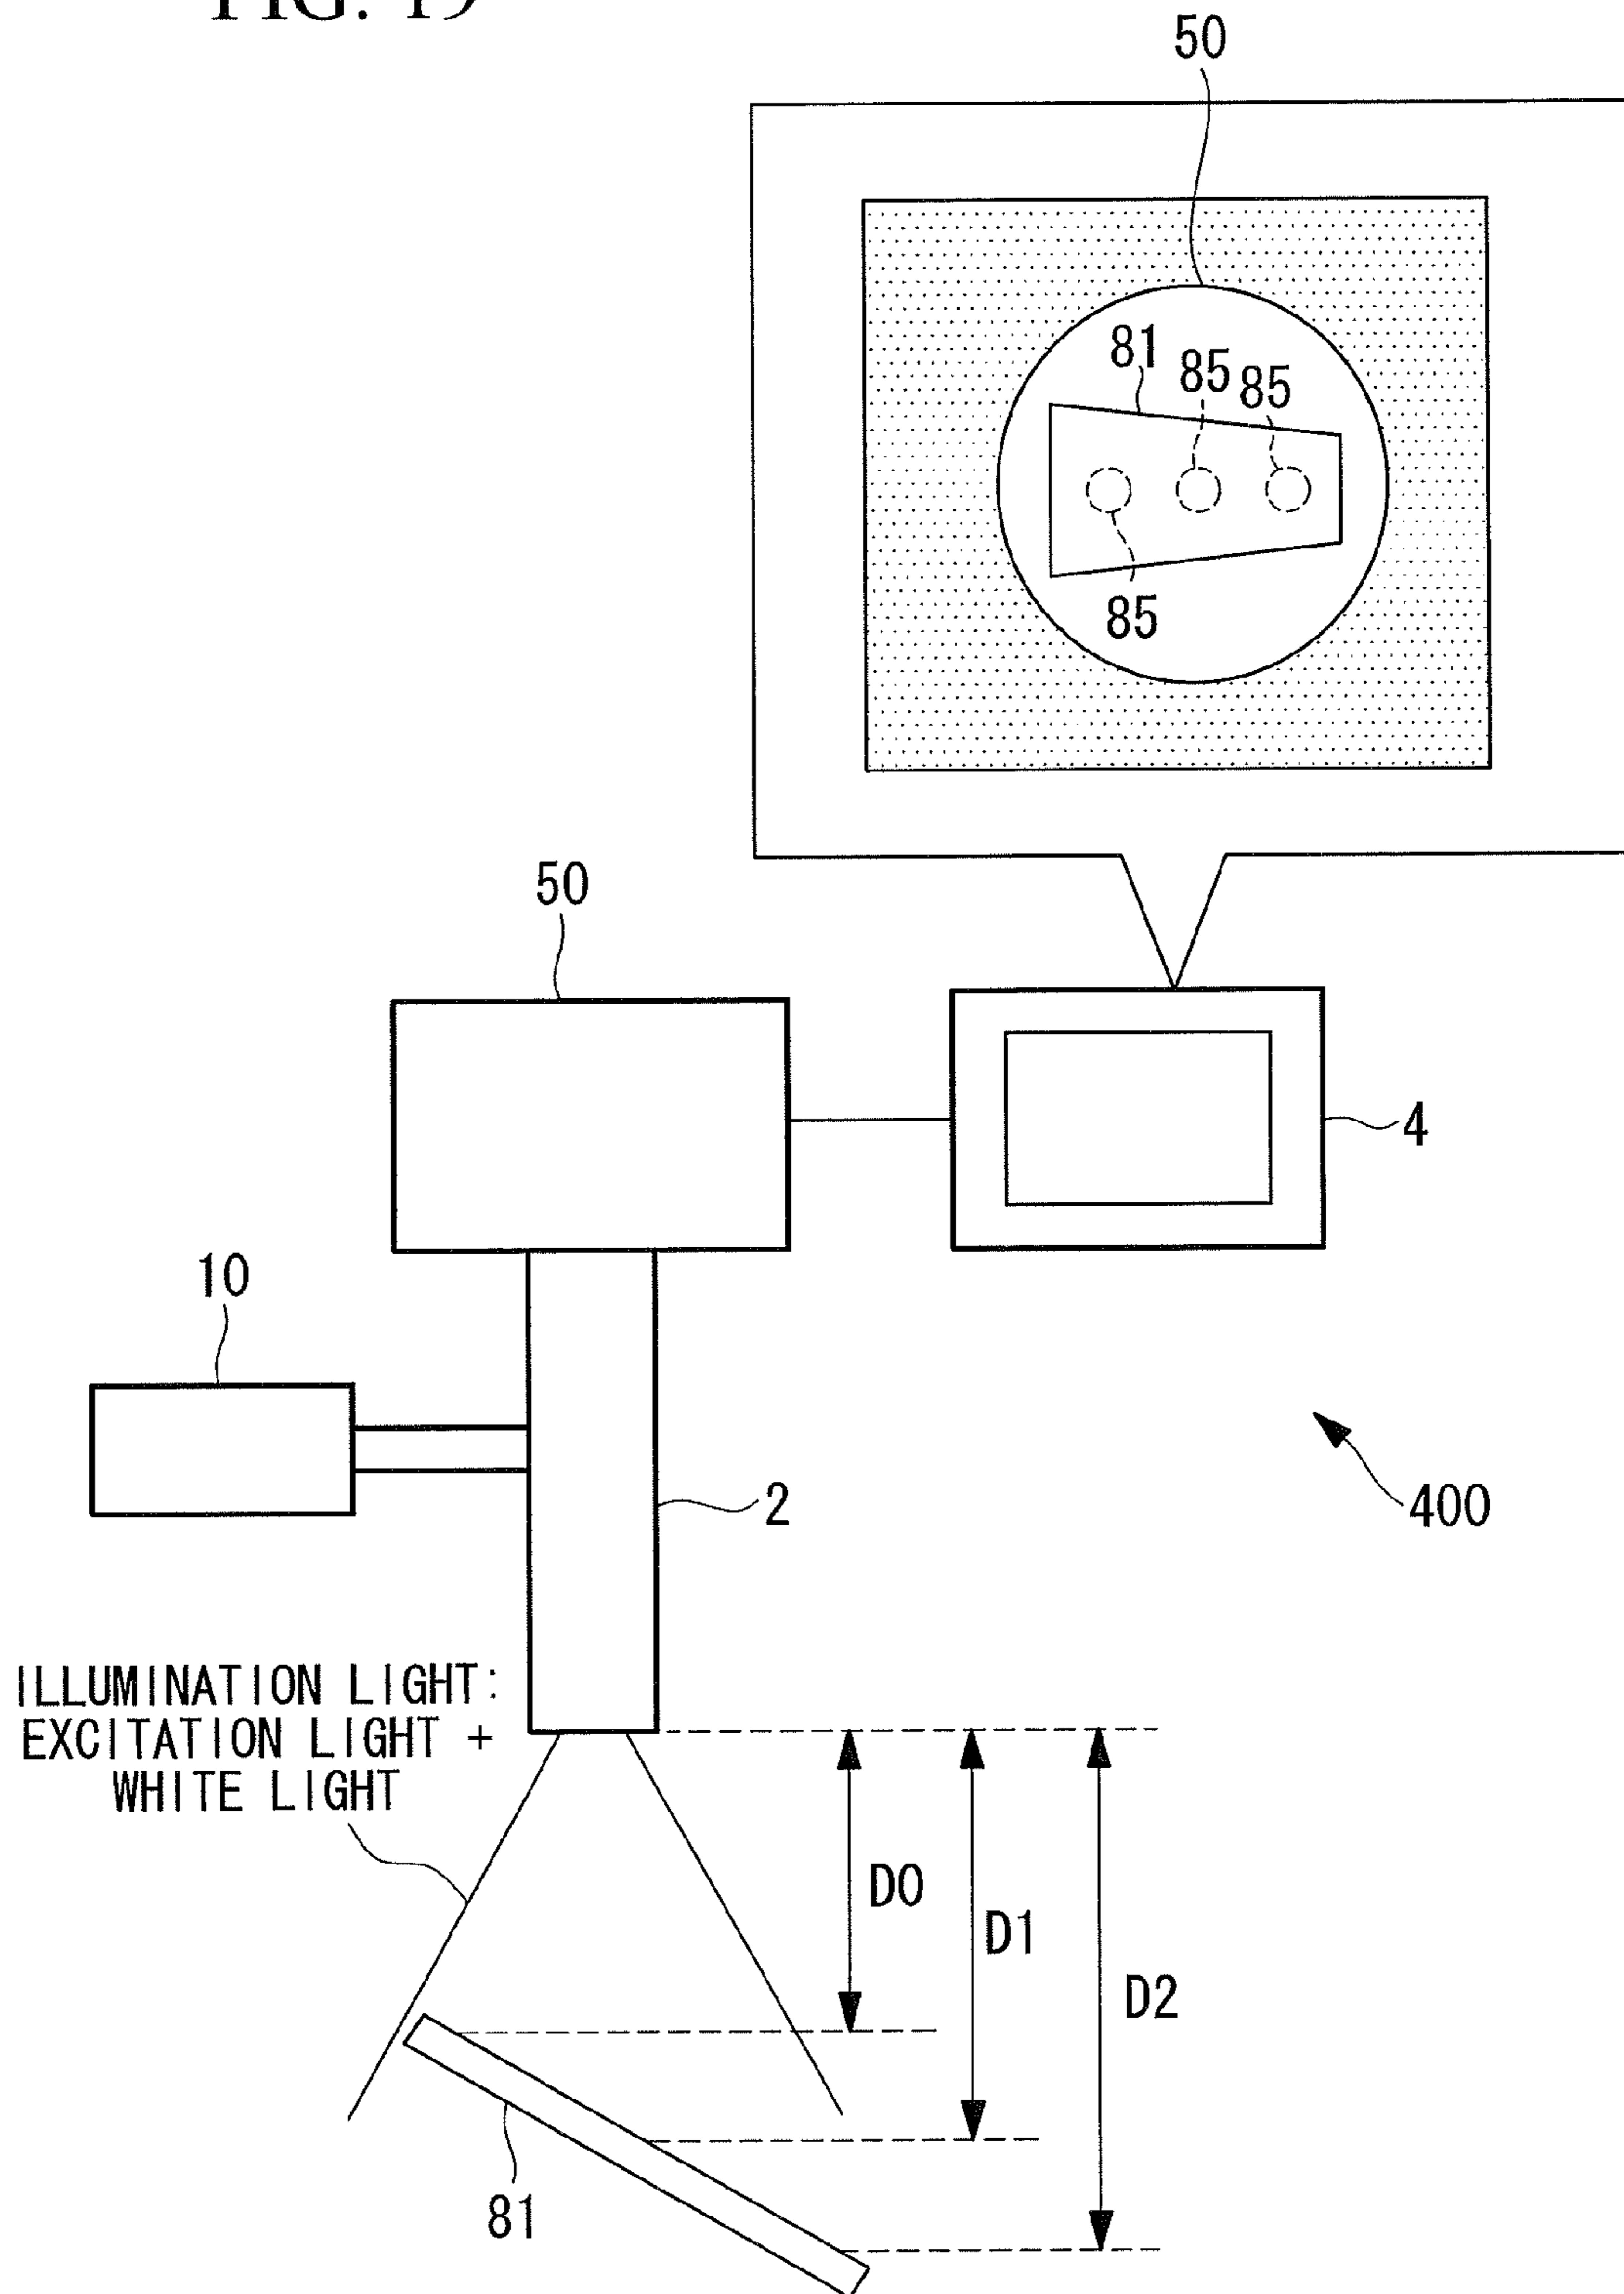


FIG. 20

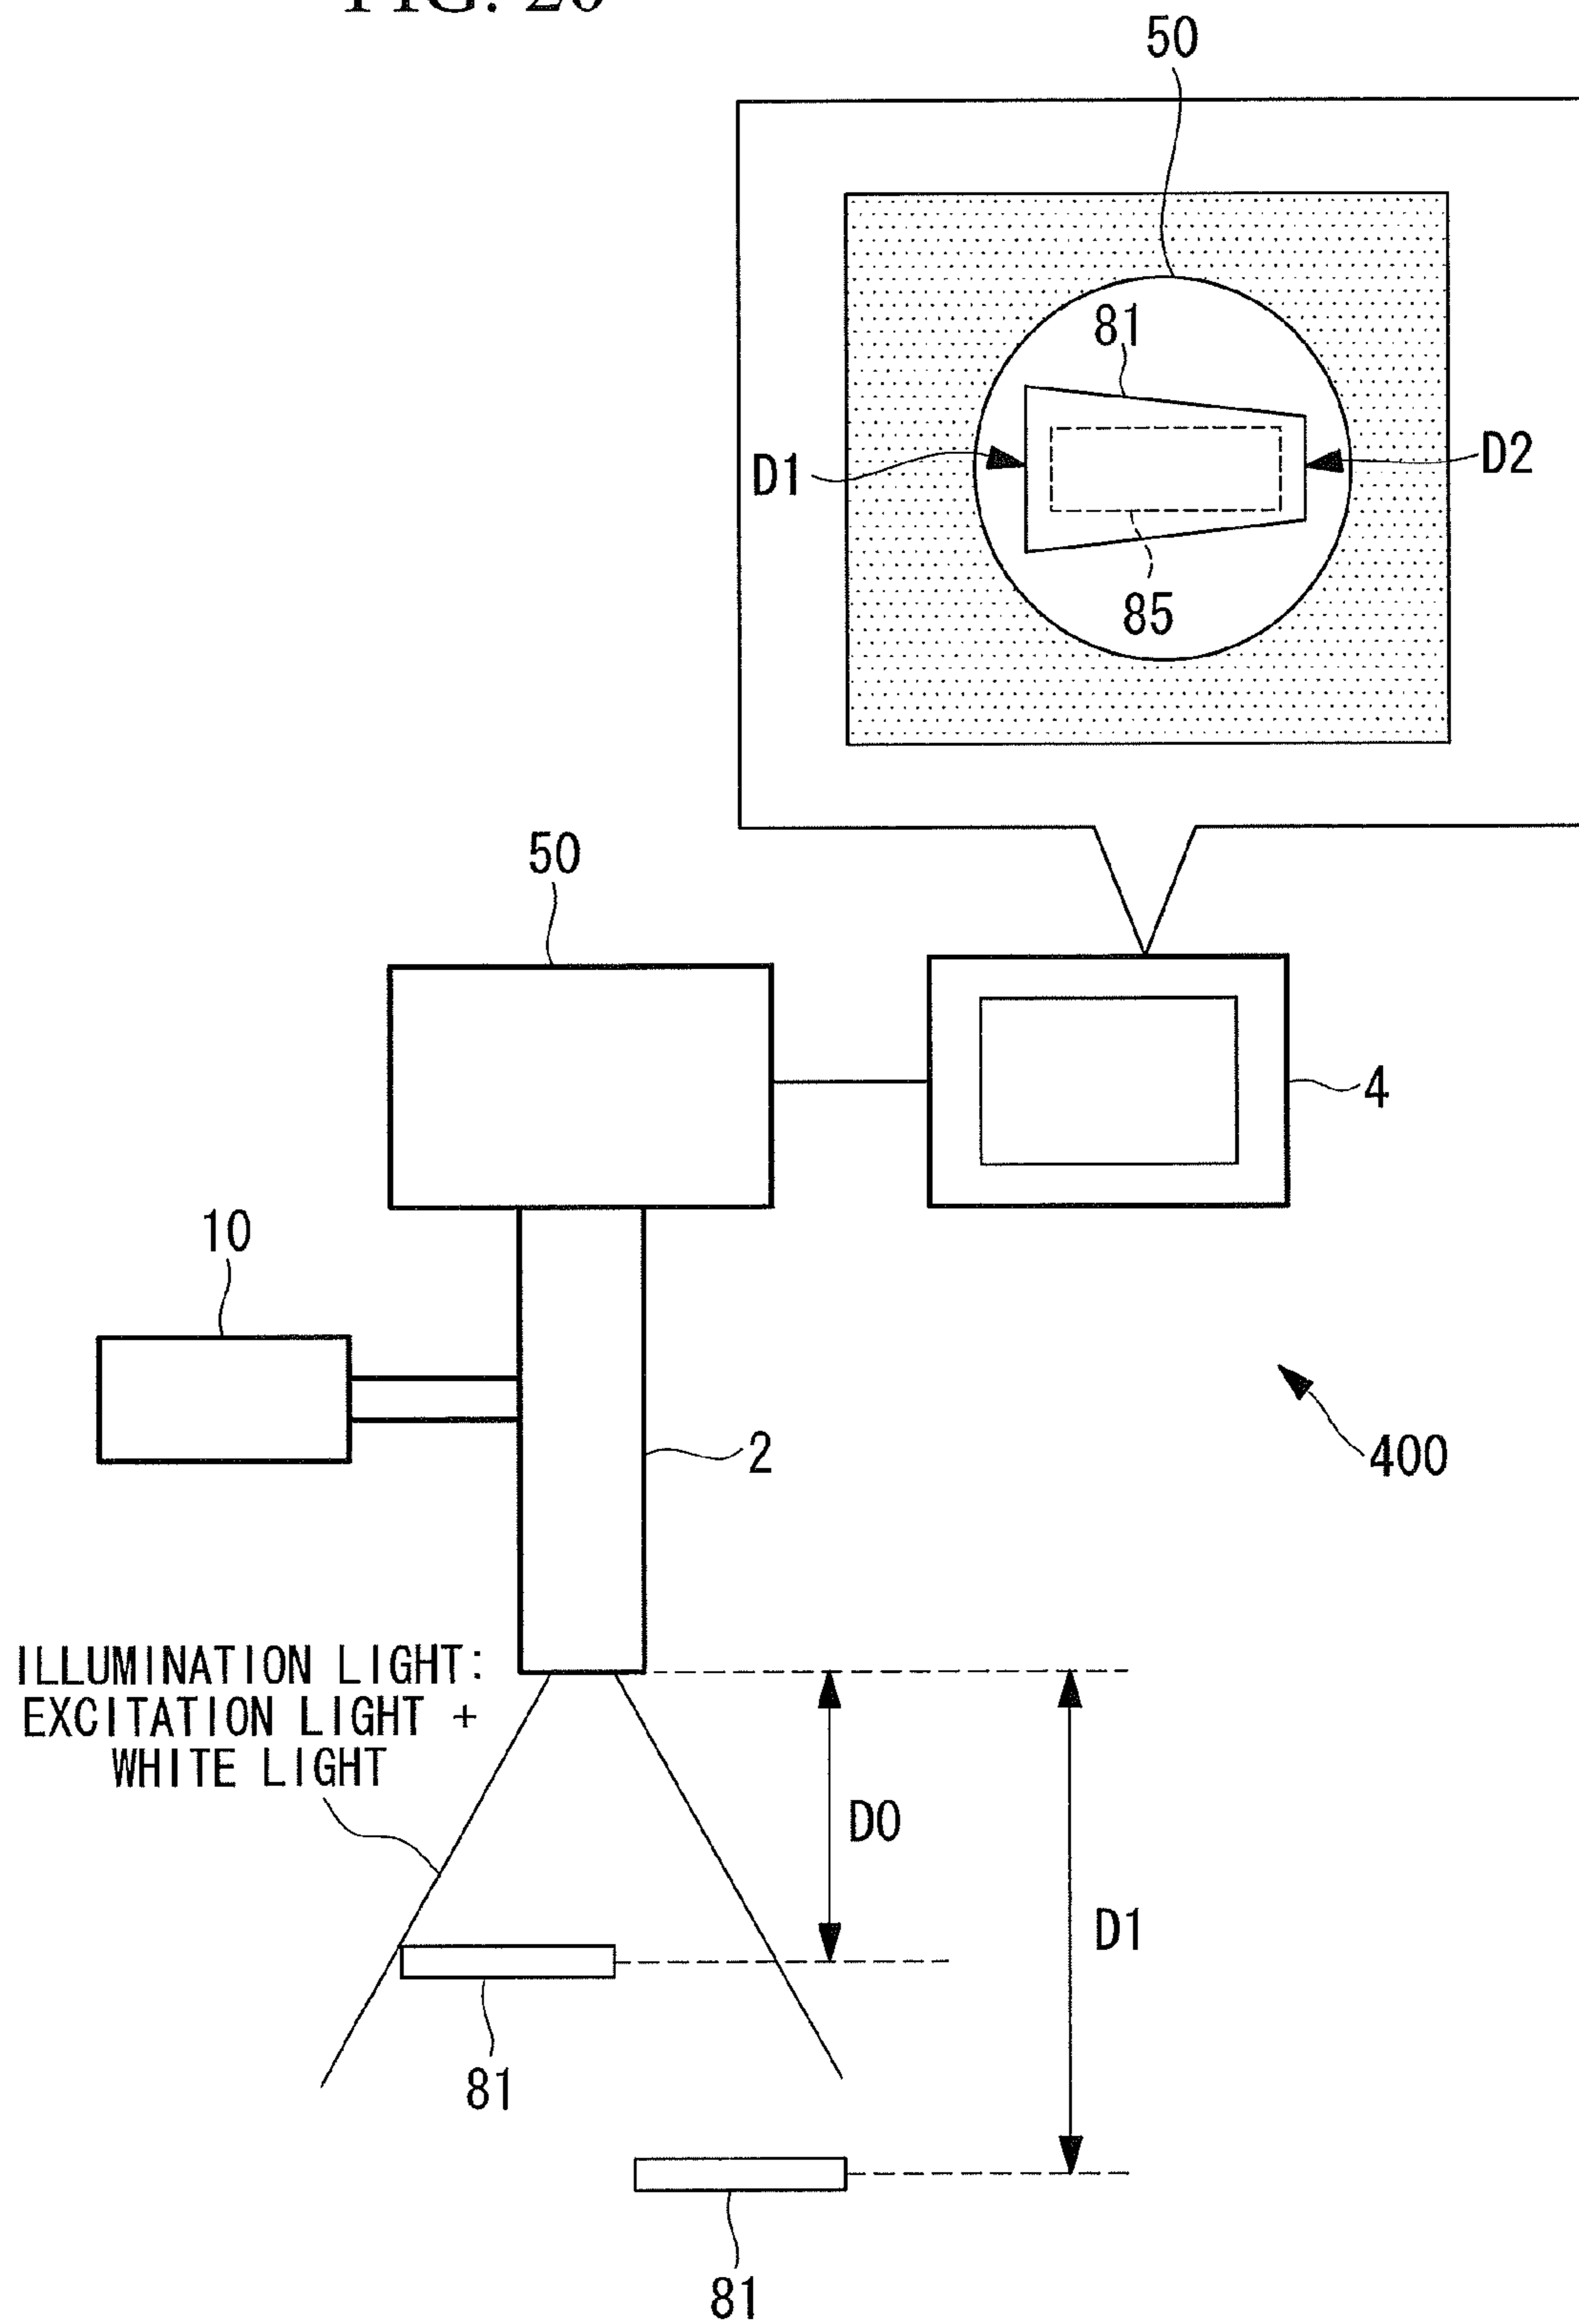


FIG. 21

CORRECTION FACTOR a	STANDARD DEVIATION σ OF FL/RL ^a IN REGION OF INTEREST
1 (NO CORRECTION)	1
0.95	0.95
⋮	⋮
0.5	0.5

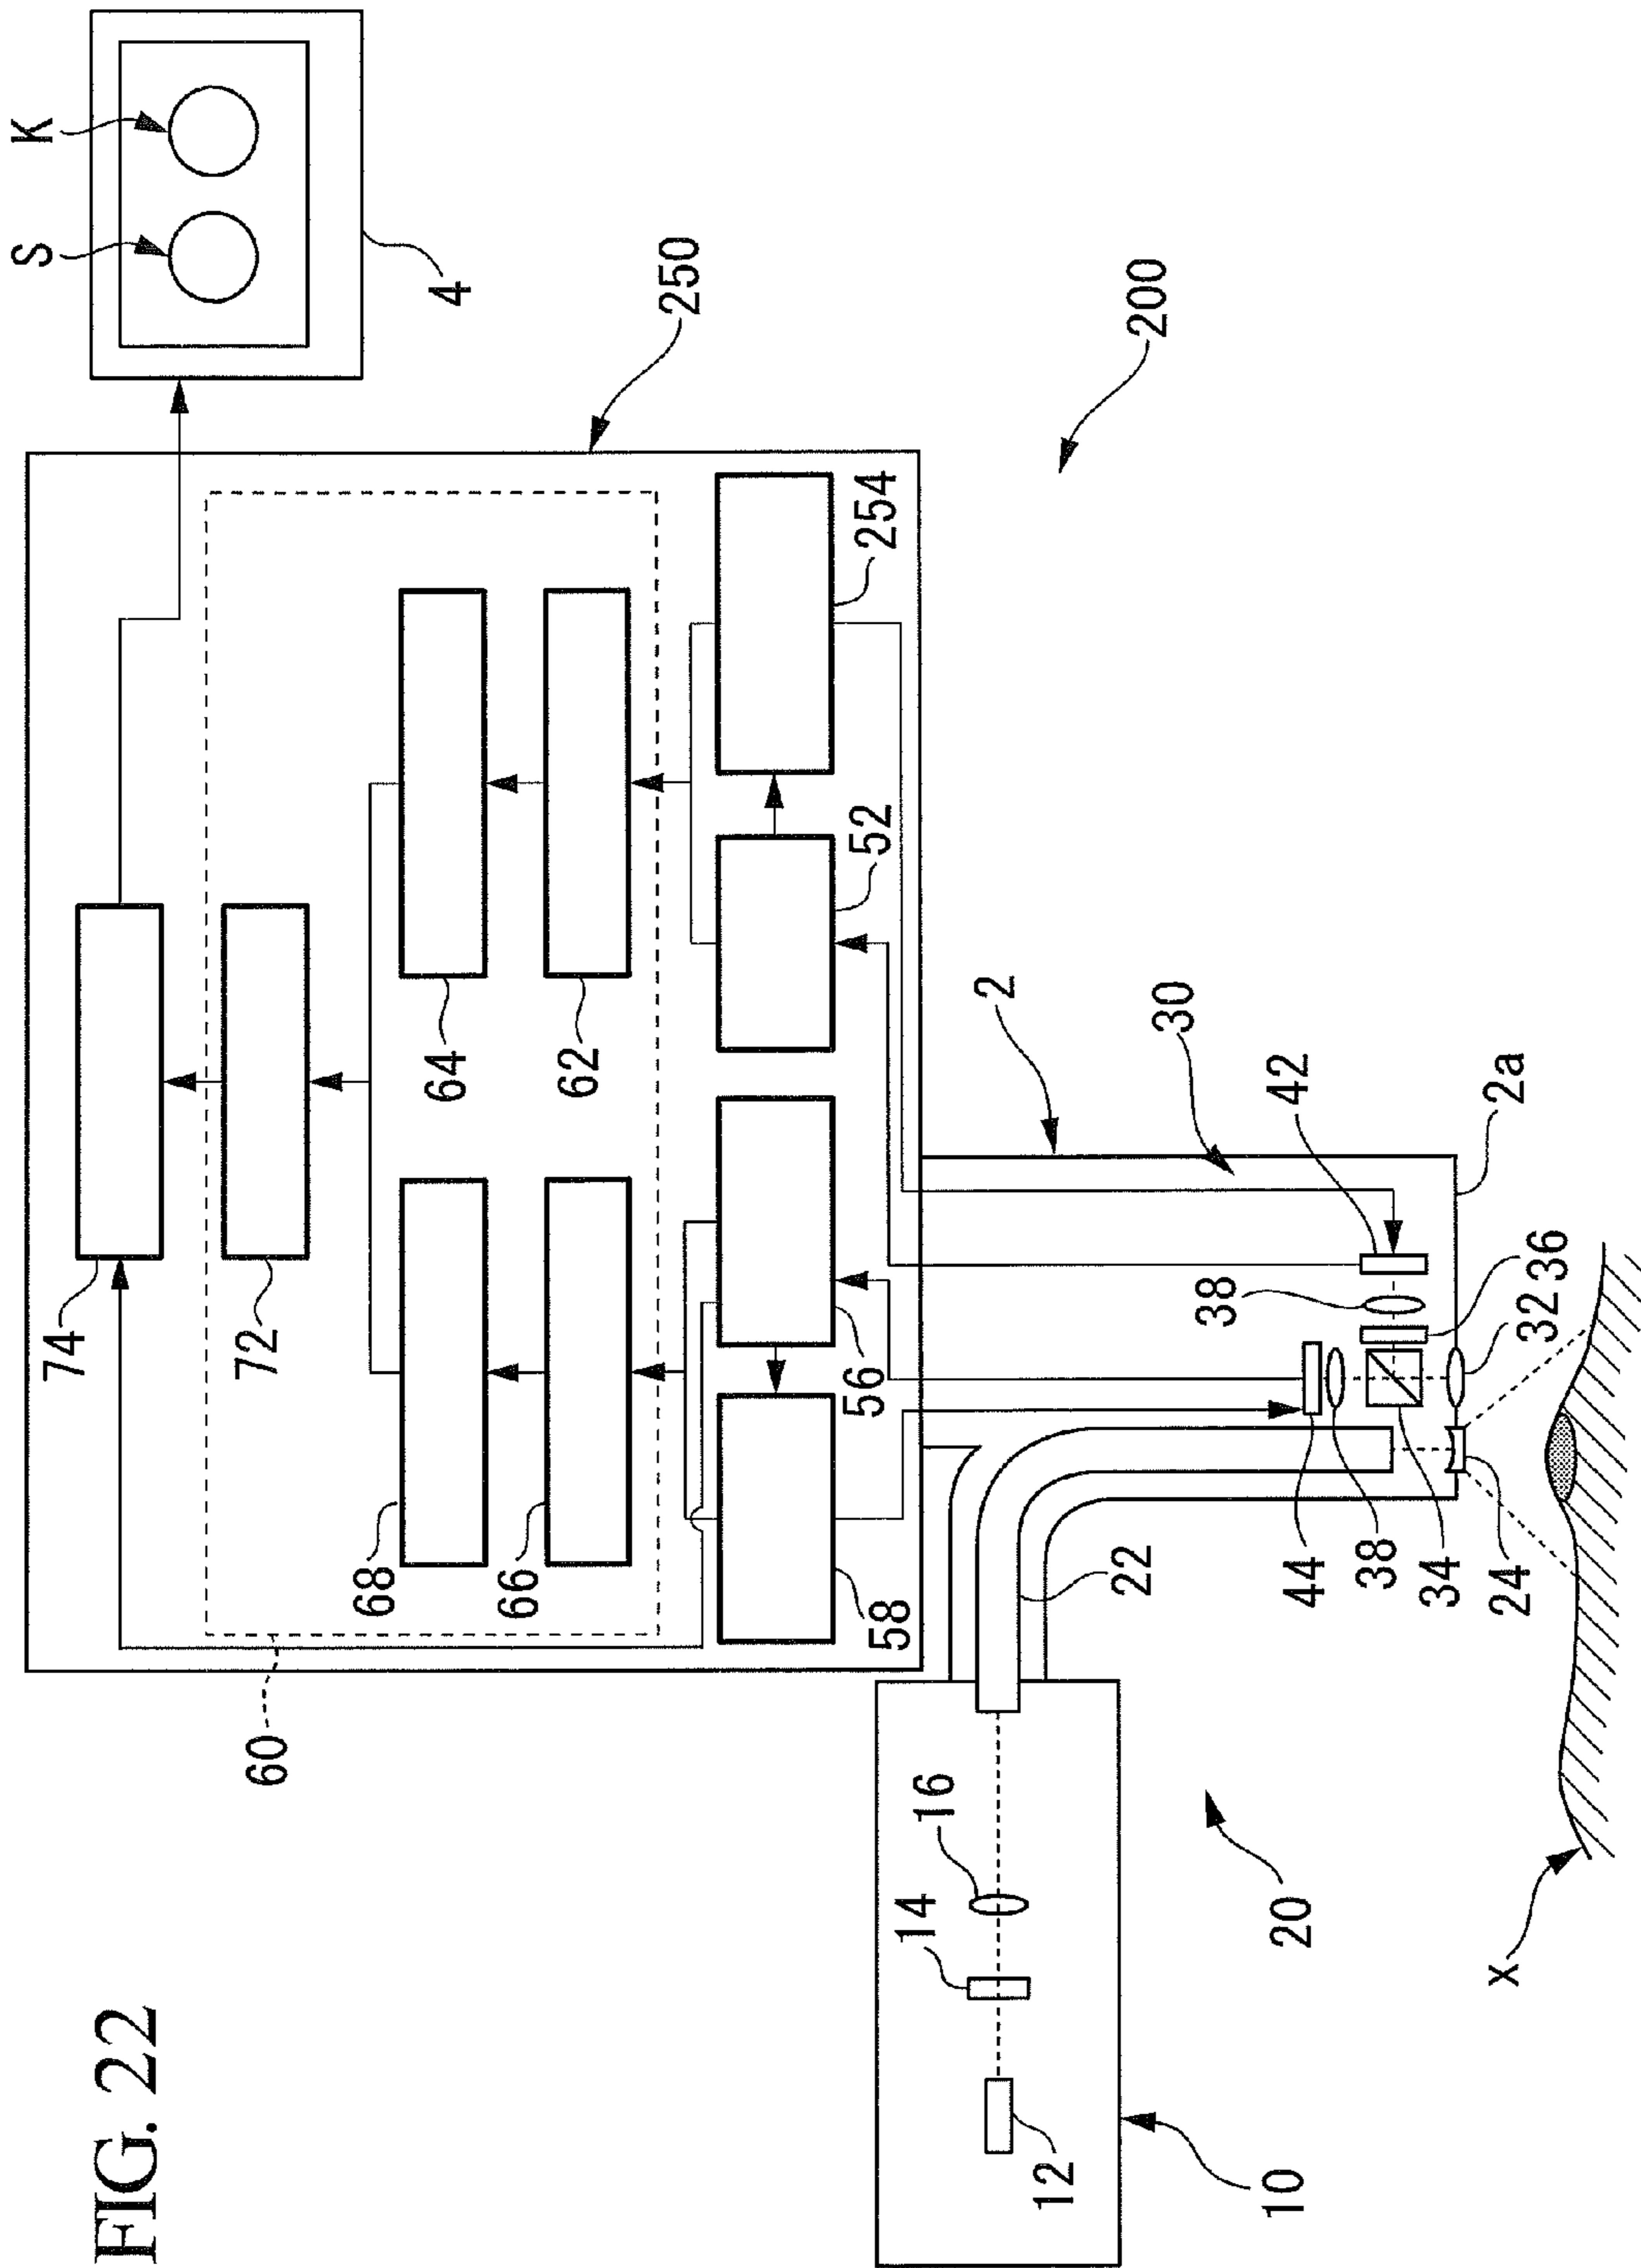


FIG. 23

GAIN VALUE	GAIN MULTIPLICATION FACTOR (FG)
0	1
1	2
⋮	⋮
8	50


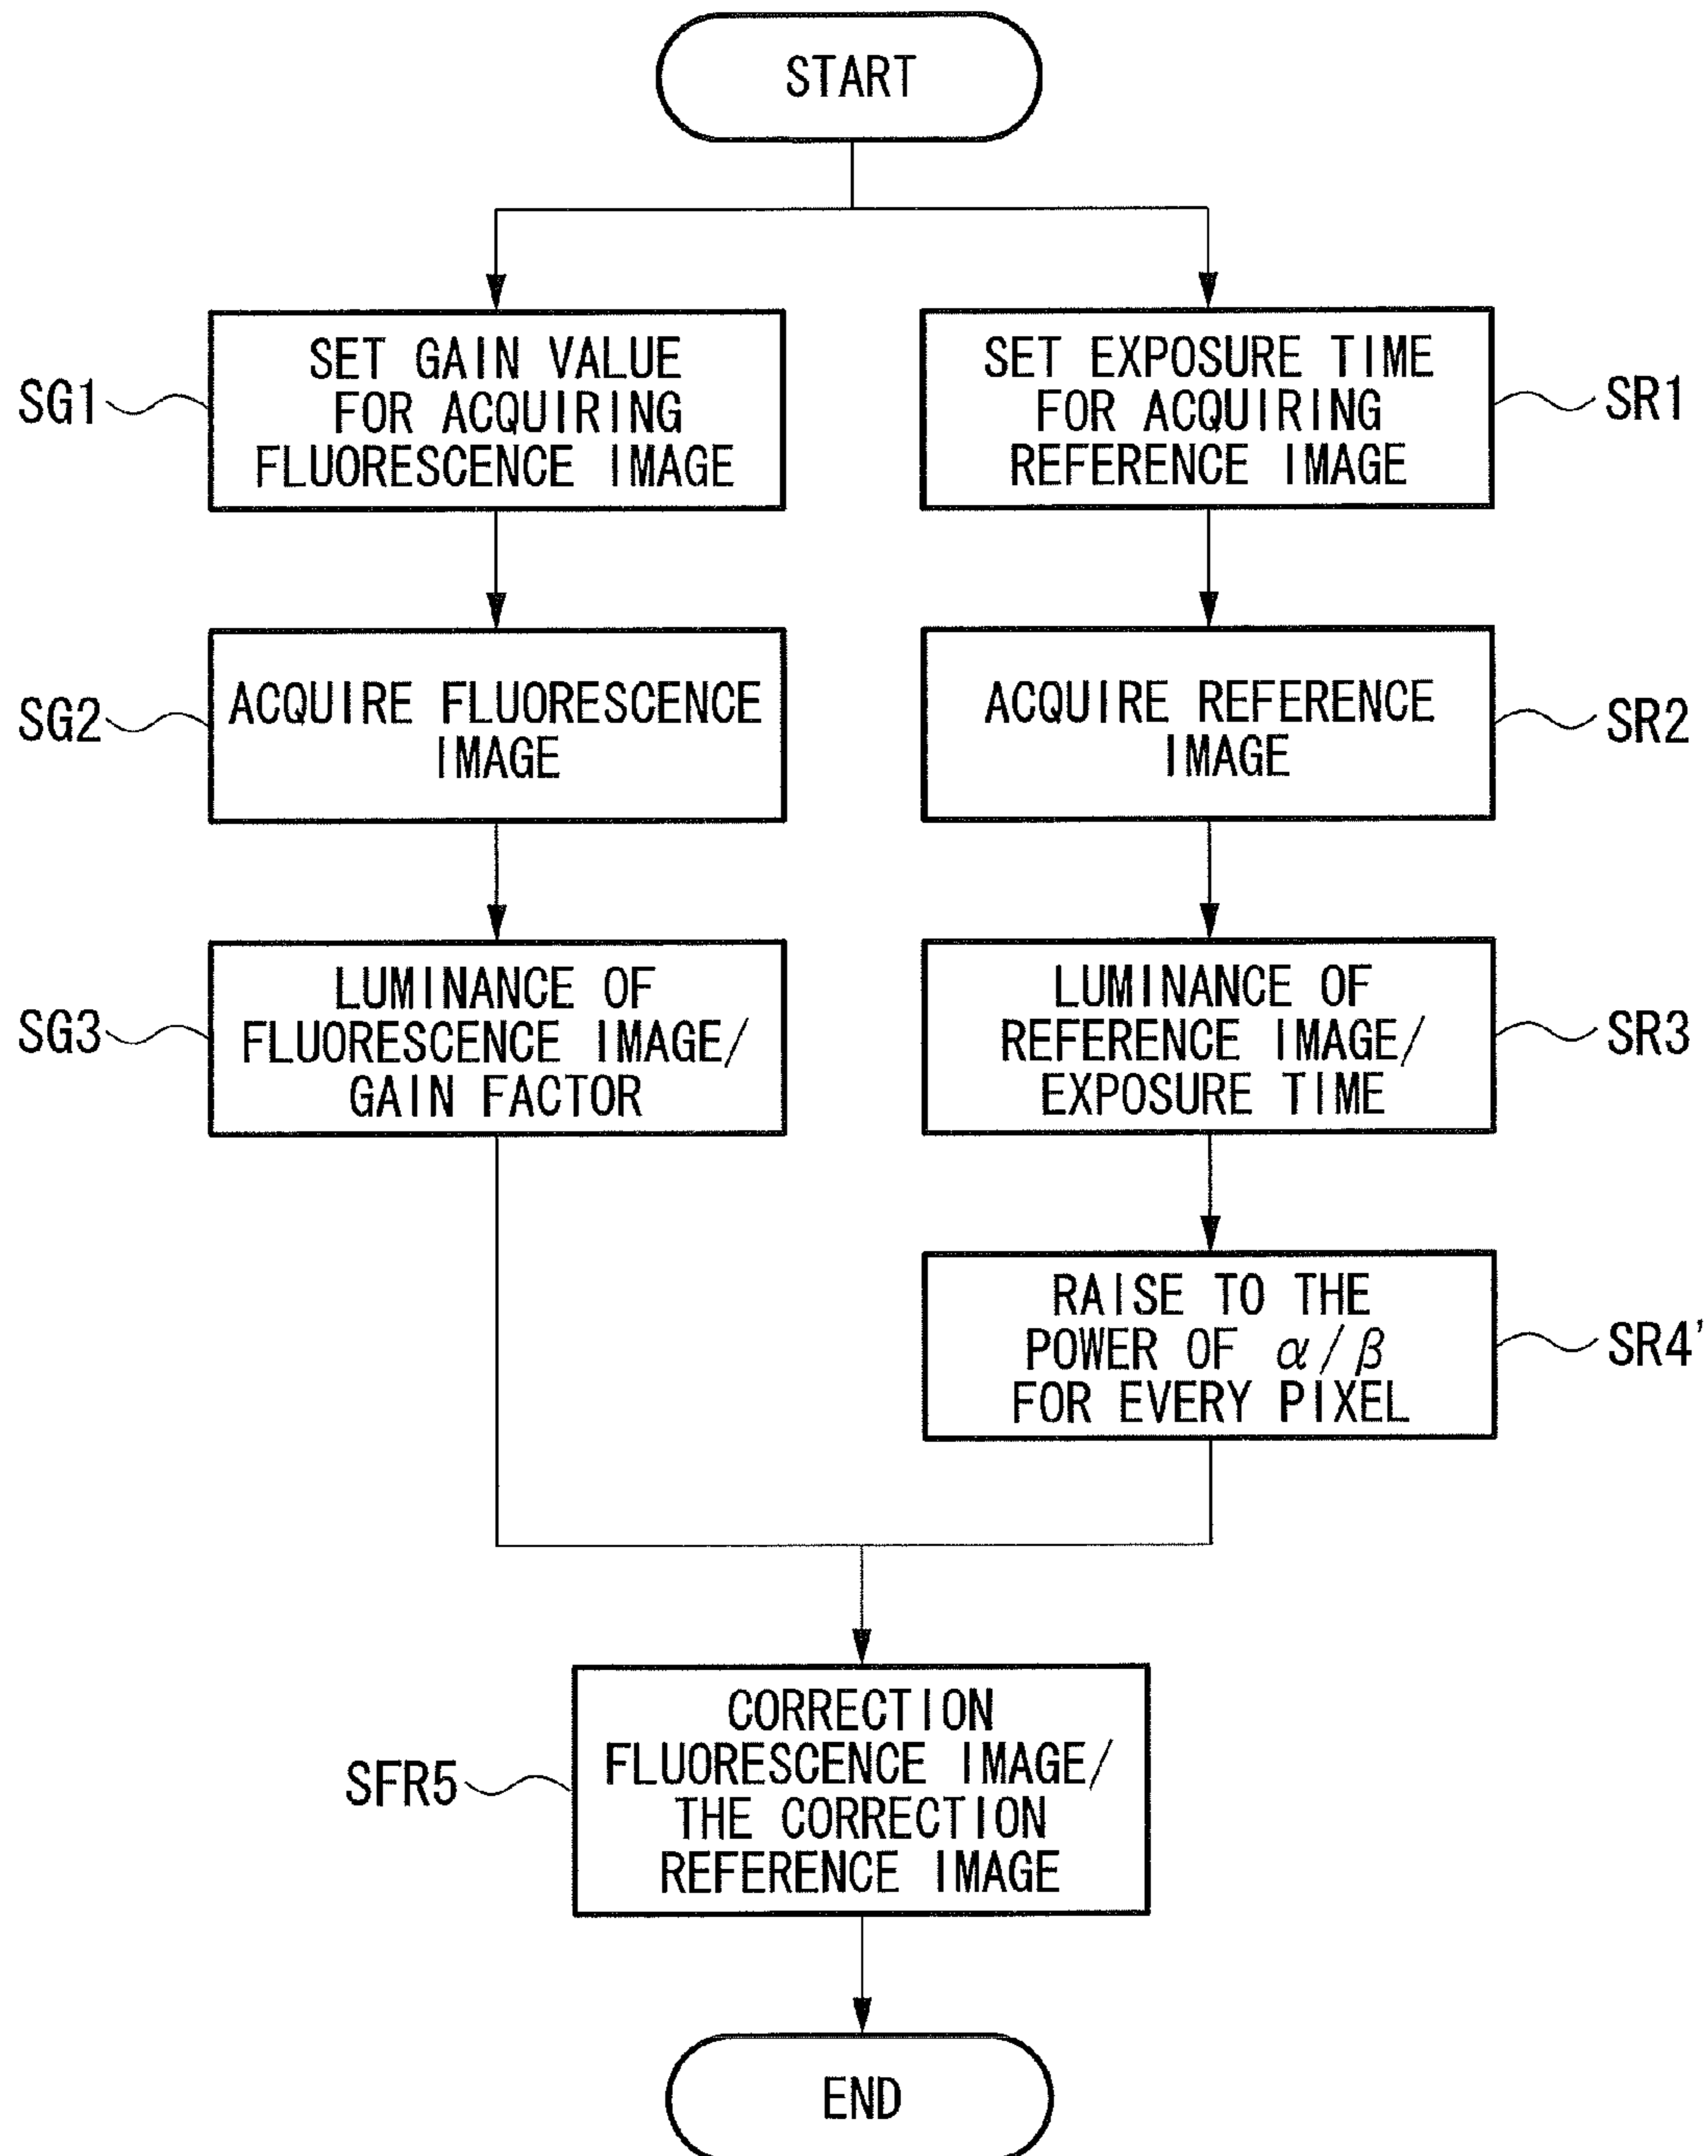
287


FIG. 24



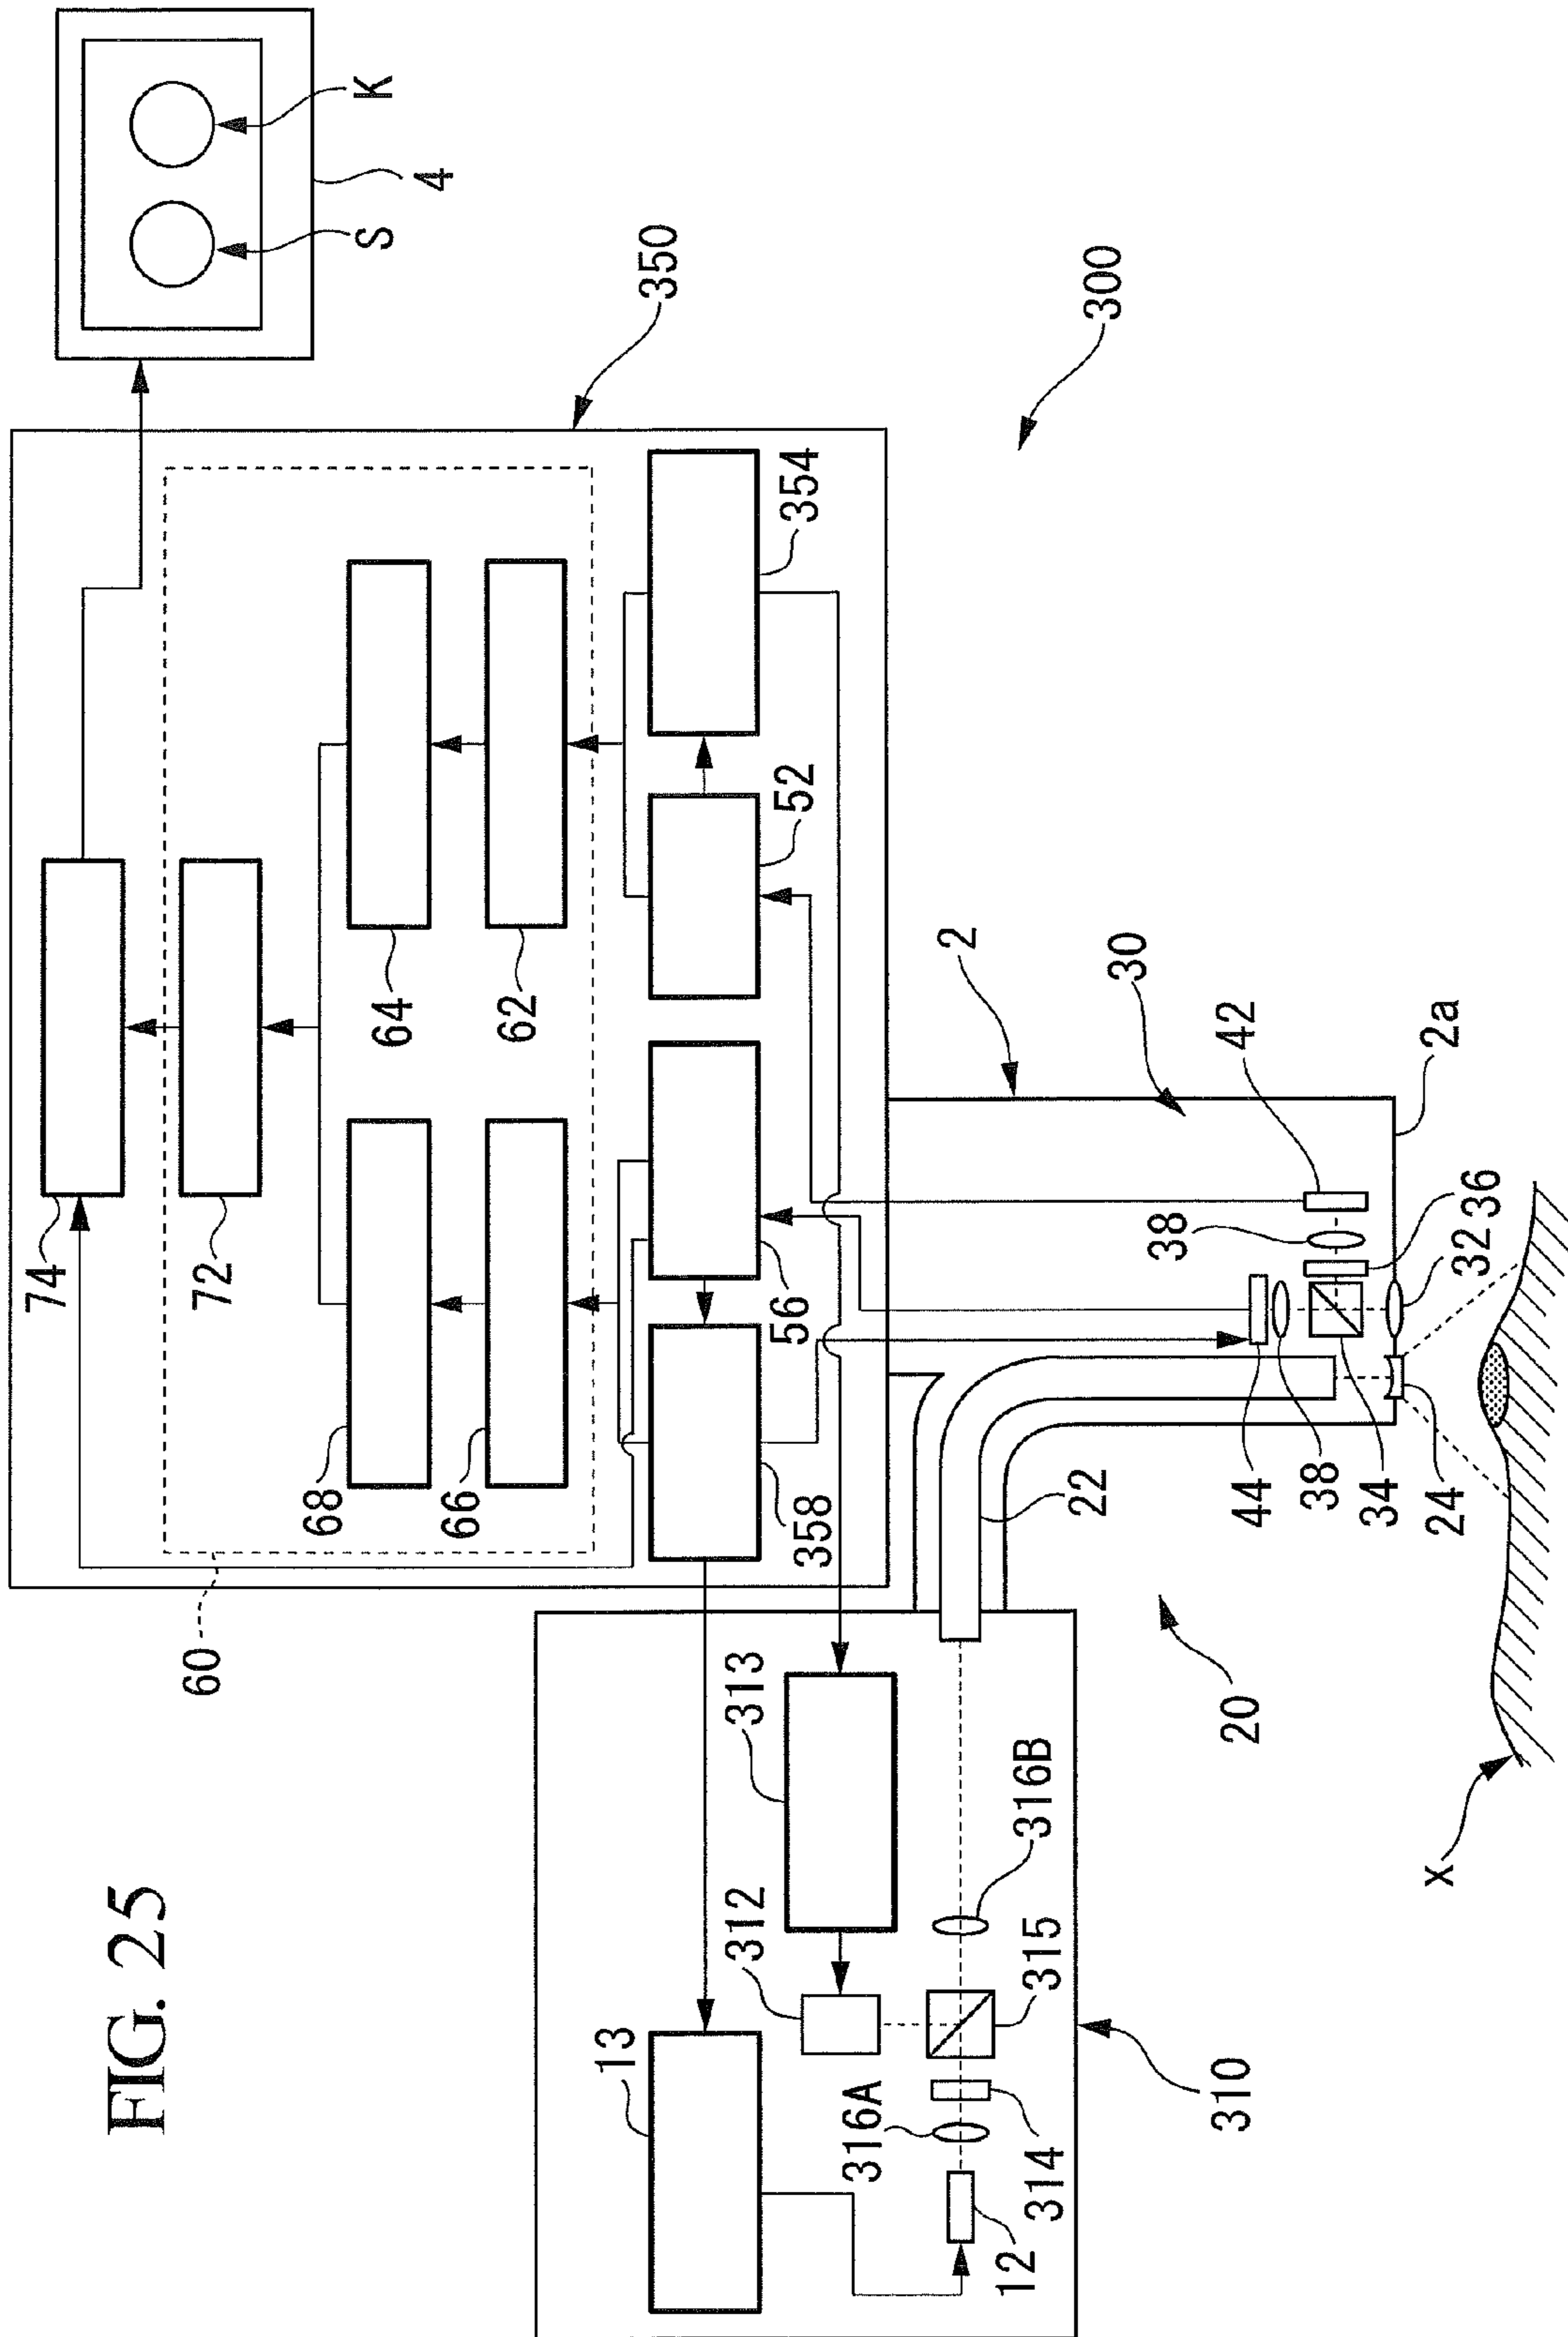


FIG. 25


FIG. 26

LIGHT-ADJUSTMENT LEVEL	EXCITATION LIGHT INTENSITY
0	1
1	2
⋮	⋮
8	50

387

An arrow originates from the number 387 and points towards the table structure.

FIG. 27

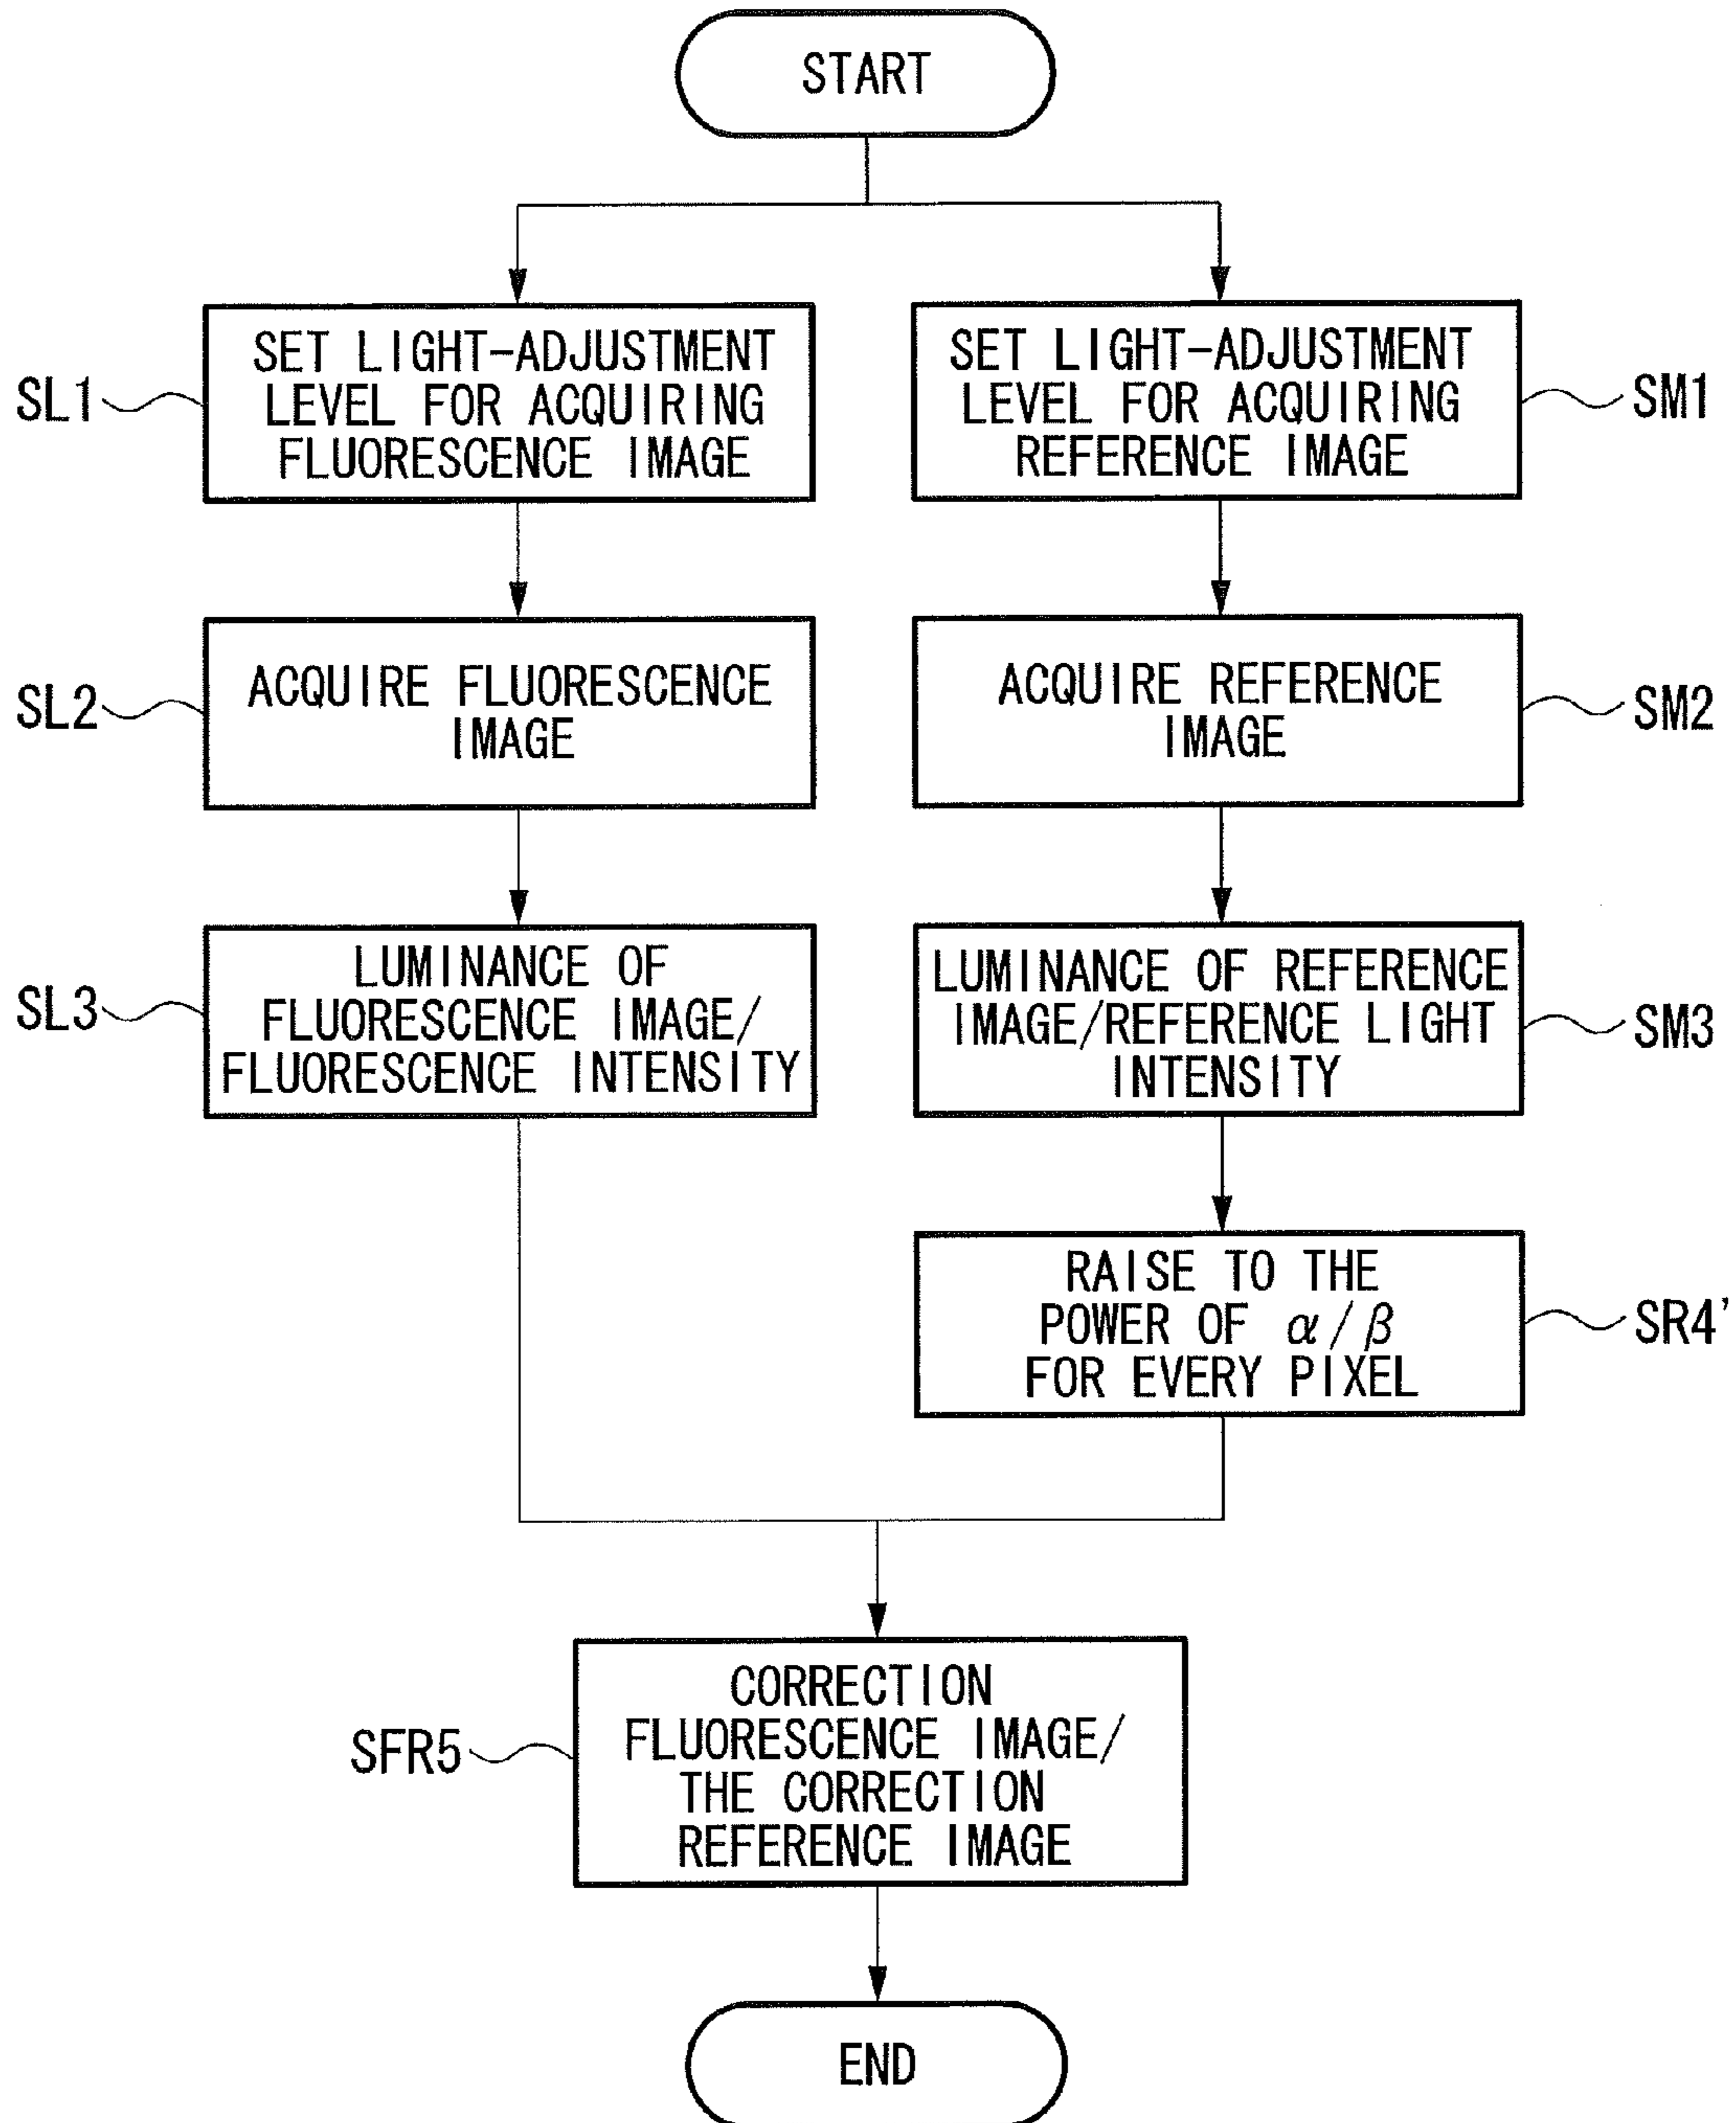

1

**FLUOROSCOPY APPARATUS,
FLUOROSCOPY SYSTEM, AND
FLUORESCENCE-IMAGE PROCESSING
METHOD**

CROSS REFERENCE TO RELATED
APPLICATIONS

This application is a divisional application of U.S. Ser. No. 13/235,886 filed Sep. 19, 2011, which is a continuation of International Application PCT/JP2010/054510, with an international filing date of Mar. 17, 2010, each of which are incorporated by reference herein in their entirety. This application claims the benefit of Japanese Patent Application No. 2009-072852, the content of which is incorporated herein by reference.

TECHNICAL FIELD

The present invention relates to a fluoroscopy apparatus, a fluoroscopy system, and a fluorescence-image processing method.

BACKGROUND ART

In the related art, there is a known fluoroscopy apparatus that is capable of obtaining a high-luminance fluorescence image of a lesion by radiating excitation light, which excites fluorescent dye to generate agent-fluorescence, onto an observation target site, to which a fluorescent dye that specifically accumulates at a lesion, such as cancer cells, is administered, and by capturing the agent-fluorescence generated (for example, see Patent Literature 1).

In the fluoroscopy apparatus described in Patent Literature 1, since the intensity of the excitation light radiated onto an observation target site varies depending on distance, in order to correct the influence due to the distance, arithmetic processing in which a fluorescence image of the observation target site is divided by a reflected-light image of the same observation target site is performed.

CITATION LIST

Patent Literature

{PTL 1} Japanese Unexamined Patent Application, Publication No. Sho 62-247232.

SUMMARY

The present invention employs the following solutions.

A first aspect of the present invention is a fluoroscopy apparatus including, an illumination portion having a light source that radiates illumination light and excitation light onto a subject, a fluorescence-imaging unit that acquires a fluorescence image by imaging fluorescence generated at the subject by the radiation of the excitation light from the illumination portion, a return-light imaging unit that acquires a reference image by imaging return light returning from the subject by the radiation of the illumination light from the illumination portion, and an image-correction unit that corrects the fluorescence image acquired by the fluorescence-imaging unit by using the reference image acquired by the return-light imaging unit, wherein in the image-correction unit, a correction fluorescence image is obtained by raising a luminance value of the fluorescence image to the power of the reciprocal of a first exponent that is obtained by a power

2

approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image acquired by the fluorescence-imaging unit when the excitation light of a prescribed intensity is radiated towards the subject; a correction reference image is obtained by raising a luminance value of the reference image to the power of the reciprocal of a second exponent that is obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the reference image obtained by the return-light imaging unit when the illumination light of a prescribed intensity is radiated towards the subject; and a corrected fluorescence image is obtained by dividing the correction fluorescence image by the correction reference image.

According to this aspect, by radiating the excitation light emitted from the illumination portion onto the subject, the fluorescence generated at the subject is imaged by the fluorescence-imaging unit imaging unit and a fluorescence image is acquired, and by radiating the illumination light emitted from the illumination portion together with the excitation light onto the subject, the return light thereof is imaged by the return-light imaging unit and a reference image is acquired.

In this case, the fluorescence image acquired by the fluorescence-imaging unit contains information related to the fluorescence that is raised to the power of the distance from the illumination portion to the subject, and the reference image acquired by the return-light imaging unit contains information related to the illumination light that is raised to the power of the distance from the illumination portion to the subject. In addition, because the fluorescence and return-light characteristics differ if they are influenced by internal scattering, surface reflection, or the like, the characteristic of the luminance of the fluorescence image on the distance from the illumination portion to the subject differs from the characteristic of the luminance of the reference image on the distance from the illumination portion to the subject.

According to the fluoroscopy apparatus of the present invention, in the image-correction unit, by raising the luminance value of the fluorescence image to the power of the reciprocal of the first exponent obtained by a power approximation of the characteristic of the luminance versus distance from the illumination portion to the subject, for the fluorescence image, it is possible to obtain the correction fluorescence image having a substantially constant luminance relative to variations in the distance. In addition, by raising the luminance value of the reference image to the power of the reciprocal of the second exponent obtained by a power approximation of the characteristic of the luminance of versus distance from the illumination portion to the subject, for the reference image, it is possible to obtain the correction reference image having a substantially constant luminance relative to the variations of the distance. Therefore, by dividing the correction fluorescence image by the correction reference image, it is possible to obtain a corrected fluorescence image having quantitiveness, in which the dependencies of the fluorescence image and the reference image on distance are cancelled and in which correction is achieved with high accuracy, allowing a lesion to be diagnosed accurately.

In this aspect, the image-correction unit may further raise the luminance value of the corrected fluorescence image to the power of the first exponent.

Configuring in this way, it is possible to reduce the dependency on the distance by the image-correction unit, while maintaining a direct-proportionality relationship between the luminance value of the corrected fluorescence image and the amount of the fluorescent agent present in the subject (i.e., the concentration of fluorescent agent).

A second aspect of the present invention is a fluoroscopy apparatus comprising, an illumination portion having a light source that radiates illumination light and excitation light onto a subject, a fluorescence-imaging unit that acquires a fluorescence image by imaging fluorescence generated at the subject by the radiation of the excitation light from the illumination portion, a return-light imaging unit that acquires a reference image by imaging return light returning from the subject by the radiation of the illumination light from the illumination portion, and an image-correction unit that corrects the fluorescence image acquired by the fluorescence-imaging unit by using the reference image acquired by the return-light imaging unit, wherein in the image-correction unit, a first exponent is obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image acquired by the fluorescence-imaging unit when the excitation light of a prescribed luminance is radiated towards the subject; a second exponent is obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for a reference image acquired by a return-light imaging unit when the illumination light of a prescribed intensity is radiated towards the subject; a correction reference image is obtained by raising the luminance value of the reference image to the power of a third exponent that is obtained by dividing the first exponent by the second exponent; a correction fluorescence image is obtained by dividing the fluorescence image by the correction reference image, or by raising the luminance value of the fluorescence image to the power of a fourth exponent that is obtained by dividing the second exponent by the first exponent; and a corrected fluorescence image is obtained by dividing the correction fluorescence image by the reference image.

According to this aspect, in the image-correction unit, it is sufficient to perform the power computation only once to correct the influence of the distance with high precision, and it is possible to obtain the corrected fluorescence image in which the luminance value and the amount of the fluorescent agent present have a direct-proportionality relationship.

A third aspect of the present invention is a fluoroscopy apparatus comprising, an illumination portion having a light source that radiates illumination light and excitation light onto a subject, a fluorescence-imaging unit that acquires a fluorescence image by imaging fluorescence generated at the subject by the radiation of the excitation light from the illumination portion, a return-light imaging unit that acquires a reference image by imaging return light returning from the subject by the radiation of the illumination light from the illumination portion, and an image-correction unit that corrects the fluorescence image acquired by the fluorescence-imaging unit by using the reference image acquired by the return-light imaging unit, wherein the image-correction unit obtains a correction fluorescence image by raising a luminance value of the fluorescence image to the power of the first correction factor that is obtained such that ratios of a luminance of the fluorescence image, in which the luminance value of the fluorescence image has been raised to the power of a first correction factor, to a luminance of the reference image match each other at a plurality of different distances, and obtains a corrected fluorescence image by dividing the correction fluorescence image by the reference image.

According to this aspect, only the ratios of the intensities of the luminance of the fluorescence image and of the reference light image at a plurality of different distances need to be obtained, and it is not necessary to obtain the distance information. In addition, because the distance characteristic is not

subjected to a power approximation, it is possible to decide the first correction factor with a simple computation.

A fourth aspect of the present invention is a fluoroscopy apparatus comprising, an illumination portion having a light source that radiates illumination light and excitation light onto a subject, a fluorescence-imaging unit that acquires a fluorescence image by imaging fluorescence generated at the subject by the radiation of the excitation light from the illumination portion, a return-light imaging unit that acquires a reference image by imaging return light returning from the subject by the radiation of the illumination light from the illumination portion, and an image-correction unit that corrects the fluorescence image acquired by the fluorescence-imaging unit by using the reference image acquired by the return-light imaging unit, wherein the image-correction unit obtains the correction reference image by raising a luminance value of the reference image to the power of the second correction factor that is obtained such that ratios of a luminance of the fluorescence image to a luminance of the reference image, in which the luminance value of the reference image has been raised to the power of a second correction factor, match each other at a plurality of different distances, and obtains a corrected fluorescence image by dividing the fluorescence image by the correction reference image.

According to this aspect, by deciding only the second correction factor from the luminance information of the fluorescence image and the reference image at a plurality of different distances, it is possible to easily obtain the corrected fluorescence image having high quantitiveness, in which the distance dependencies of the fluorescence image and the reference image are reduced.

A fifth aspect of the present invention is a fluoroscopy apparatus comprising, an illumination portion having a light source that radiates illumination light and excitation light onto a subject, a fluorescence-imaging unit that acquires a fluorescence image by imaging fluorescence generated at the subject by the radiation of the excitation light from the illumination portion, a return-light imaging unit that acquires a reference image by imaging return light returning from the subject by the radiation of the illumination light from the illumination portion, and an image-correction unit that corrects the fluorescence image acquired by the fluorescence-imaging unit by using the reference image acquired by the return-light imaging unit, wherein the image-correction unit obtains a correction fluorescence image by raising a luminance value of the fluorescence image to the power of the first correction factor that is obtained such that ratios of a luminance of the fluorescence image, in which the luminance value of the fluorescence image has been raised to the power of a first correction factor, to a luminance of the reference image, in which the luminance value of the reference image has been raised to the power of a second correction factor, match each other at a plurality of different distances, obtains the correction reference image by raising the luminance value of the reference image to the power of the second correction factor, and obtains a corrected fluorescence image by dividing the correction fluorescence image by the correction reference image.

According to this aspect, by deciding only two correction factors from the luminance information of the fluorescence image and the reference image at a plurality of different distances, it is possible to easily obtain a corrected fluorescence image having high quantitiveness in which the distance dependencies of the fluorescence image and the reference image are reduced.

In the above-described aspect, an image-acquisition condition adjusting portion that adjusts an image acquisition

5

condition on the basis of the luminance value of the fluorescence image acquired by the fluorescence-imaging unit, may be provided, wherein the image-correction unit may normalize the luminance of the fluorescence image by the image acquisition condition.

Configuring in this way, it is possible to obtain a fluorescence image having suitable brightness with the image-acquisition condition adjusting portion regardless of the luminance of the fluorescence generated at the subject. In this case, by normalizing the luminance of the fluorescence image by the image acquisition condition with the image-correction unit, it is possible to standardize the luminance value of the fluorescence image even when the image acquisition condition of the image-acquisition condition adjusting portion is changed.

In the above-described aspect, the image-acquisition condition adjusting portion may adjust exposure time of the fluorescence-imaging unit, and the image-correction unit may divide the luminance value of the fluorescence image by the exposure time.

Configuring in this way, it is possible to adjust the brightness of the fluorescence image by using the image-acquisition condition adjusting portion by changing the exposure time of the fluorescence-imaging unit. In addition, even if the exposure time of the fluorescence-imaging unit is changed, it is possible to standardize the fluorescence image at a luminance value per unit time with the image-correction unit.

In the above-described aspect, the image-acquisition condition adjusting portion may adjust a gain factor of the fluorescence-imaging unit, and the image-correction unit may divide the luminance value of the fluorescence image by the gain factor.

Configuring in this way, it is possible to adjust the brightness of the fluorescence image by using the image-acquisition condition adjusting portion by changing the gain factor of the fluorescence-imaging unit. In addition, even if the gain factor of the fluorescence-imaging unit is changed, it is possible to standardize the fluorescence image at a certain luminance value per multiplication value with the image-correction unit.

In the above-described aspect, the image-acquisition condition adjusting portion may adjust excitation-light intensity from the illumination portion, and the image-correction unit may divide the luminance value of the fluorescence image by the excitation-light intensity.

Configuring in this way, it is possible to adjust the brightness of the fluorescence image by using the image-acquisition condition adjusting portion by changing the intensity of the excitation light radiated on the subject. In addition, even if the excitation-light intensity from the illumination portion is changed, it is possible to standardize the fluorescence image at a certain luminance value per excitation-light intensity with the image-correction unit.

In the above-described aspect, an image-acquisition condition adjusting portion that adjusts the image acquisition condition on the basis of the luminance value of the reference image acquired by the return-light imaging unit is provided, wherein the image-correction unit may normalize the luminance of the reference image by the image acquisition condition.

Configuring in this way, it is possible to obtain a reference image having suitable brightness by using the image-acquisition condition adjusting portion regardless of the luminance of the return light returning from the subject. In this case, by normalizing the luminance of the reference image by the image acquisition condition with the image-correction unit, even when the image acquisition condition of the image-

6

acquisition condition adjusting portion is changed, it is possible to standardize the luminance value of the reference image.

In the above-described aspect, the image-acquisition condition adjusting portion may adjust exposure time of the return-light imaging unit, and the image-correction unit divides the luminance value of the reference image by the exposure time.

Configuring in this way, it is possible to adjust the brightness of the reference image by changing the exposure time of the return-light imaging unit with the image-acquisition condition adjusting portion. In addition, even if the exposure time of the return-light imaging unit is changed, it is possible to standardize the reference image at a luminance value per unit time with the image-correction unit.

In the above-described aspect, the image-acquisition condition adjusting portion may adjust a gain factor of the return-light imaging unit, and the image-correction unit may divide the luminance value of the reference image by the gain factor.

Configuring in this way, it is possible to adjust the brightness of the reference image by changing the gain factor of the return-light imaging unit with the image-acquisition condition adjusting portion. In addition, even if the gain factor of the return-light imaging unit is changed, it is possible to standardize the reference image at a certain luminance value per multiplication value with the image-correction unit.

In the above-described aspect, the image-acquisition condition adjusting portion adjusts illumination light intensity from the illumination portion, and the image-correction unit divides the luminance value of the reference image by the illumination light intensity.

Configuring in this way, it is possible to adjust the brightness of the reference image by using the image-acquisition condition adjusting portion by changing the intensity of the return light returning from the subject. In addition, even if the illumination light intensity from the illumination portion is changed, it is possible to standardize the reference image at a certain luminance value per unit of illumination light intensity with the image-correction unit.

A sixth aspect of the present invention is a fluoroscopy system comprising a fluoroscopy apparatus according to the above-mentioned present invention and a calibration device that calibrates the fluoroscopy apparatus, wherein the calibration device is provided with a standard specimen and an observation-state setting mechanism that changeably sets an observation distance of the fluoroscopy apparatus relative to the standard specimen, and wherein the fluoroscopy apparatus or the calibration device is provided with an exponent calculating unit that calculates the first exponent and the second exponent on the basis of the observation distance set by the observation-state setting mechanism and the fluorescence image and the reference image acquired by imaging the standard specimen with the fluoroscopy apparatus.

According to this aspect, by calibrating the fluoroscopy apparatus with the calibration device prior to the fluorescence observation, it is possible to calculate the first exponent and the second exponent in the fluoroscopy apparatus more precisely by the operation of the exponent calculating unit on the basis of the image acquired using the standard specimen.

A seventh aspect of the present invention is a fluoroscopy system comprising a fluoroscopy apparatus according to the above-mentioned present invention and a calibration device that calibrates the fluoroscopy apparatus, wherein the calibration device is provided with a standard specimen and an observation-state setting mechanism that changeably sets an observation distance of the fluoroscopy apparatus relative to the standard specimen, and wherein the fluoroscopy appara-

tus or the calibration device is provided with a correction-factor calculating unit that calculates the first correction factor and the second correction factor on the basis of the observation distance set by the observation-state setting mechanism and the fluorescence image and the reference image acquired by imaging the standard specimen with the fluoroscopy apparatus.

According to this aspect, by calibrating the fluoroscopy apparatus with the calibration device prior to the fluorescence observation, it is possible to calculate the first correction factor and the second correction factor in the fluoroscopy apparatus more precisely by the operation of the exponent calculating unit on the basis of the image acquired using the standard specimen.

An eighth aspect of the present invention is a fluorescence-image processing method for performing the following correction processing on a fluorescence image acquired by imaging fluorescence produced at a subject by radiating excitation light from an illumination portion onto the subject by using a reference image acquired by imaging return light returning from the subject when the subject is irradiated with illumination light from the illumination portion:

$$FL_{revised} = FL_{after} / RL_{after},$$

where,

$FL_{revised}$ is a luminance value of a fluorescence image after correction,

$$FL_{after} = A \times FL_{before}^x,$$

$$RL_{after} = B \times RL_{before}^y,$$

FL_{before} and RL_{before} before are luminance values of the acquired fluorescence image and reference image,

A and B are constants,

x is a reciprocal of an exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image obtained by radiating excitation light of a prescribed intensity onto the subject, and

y is a reciprocal of an exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the reference image obtained by radiating illumination light of a prescribed intensity onto the subject.

A ninth aspect of the present invention is a fluorescence-image processing method for performing the following correction processing on a fluorescence image acquired by imaging fluorescence produced at a subject by radiating excitation light from an illumination portion onto the subject by using a reference image acquired by imaging return light returning from the subject when the subject is irradiated with illumination light from the illumination portion:

$$FL_{revised} = (FL_{after} / RL_{after})^{1/x},$$

where,

$FL_{revised}$ is a luminance value of a fluorescence image after correction,

$$FL_{after} = A \times FL_{before}^x,$$

$$RL_{after} = B \times RL_{before}^y,$$

FL_{before} and RL_{before} are luminance values of the acquired fluorescence image and reference image,

A and B are constants,

x is a reciprocal of an exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image obtained by radiating excitation light of a prescribed intensity onto the subject, and

y is a reciprocal of an exponent obtained by a power approximation of a characteristic of luminance versus dis-

tance from the illumination portion to the subject, for the reference image obtained by radiating illumination light of a prescribed intensity onto the subject.

A tenth aspect of the present invention is a fluorescence-image processing method for performing the following correction processing on a fluorescence image acquired by imaging fluorescence produced at a subject by radiating excitation light from an illumination portion onto the subject by using a reference image acquired by imaging return light returning from the subject when the subject is irradiated with illumination light from the illumination portion:

$$FL_{revised} = FL_{before} / RL_{after},$$

where,

$FL_{revised}$ is a luminance value of a fluorescence image after correction,

$$RL_{after} = B \times RL_{before}^y,$$

FL_{before} and RL_{before} before are luminance values of the acquired fluorescence image and reference image,

B is a constant;

y is a value obtained by dividing a first exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image obtained by radiating excitation light of a prescribed intensity onto the subject, by a second exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the reference image obtained by radiating illumination light of a prescribed intensity onto the subject.

An eleventh aspect of the present invention is a fluorescence-image processing method for performing the following correction processing on a fluorescence image acquired by imaging fluorescence produced at a subject by radiating excitation light from an illumination portion onto the subject by using a reference image acquired by imaging return light returning from the subject when the subject is irradiated with illumination light from the illumination portion:

$$FL_{revised} = FL_{after} / RL_{before},$$

where,

$FL_{revised}$ is a luminance value of a fluorescence image after correction,

$$FL_{after} = B \times FL_{before}^{1/y},$$

FL_{before} and RL_{before} before are luminance values of the acquired fluorescence image and reference image,

B is a constant,

y is a value obtained by dividing a first exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image obtained by radiating excitation light of a prescribed intensity onto the subject, by a second exponent obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the reference image obtained by radiating illumination light of a prescribed intensity onto the subject.

BRIEF DESCRIPTION OF DRAWINGS

FIG. 1 is a block diagram showing, in outline, the configuration of a fluoroscopy apparatus according to a first embodiment of the present invention.

FIG. 2 is a diagram showing a state in which the observation distance between an insertion portion of the fluoroscopy apparatus in FIG. 1 and a standard specimen is changed.

FIG. 3 is a flowchart showing a method of calculating an exponent in the fluoroscopy apparatus in FIG. 1.

FIG. 4A is a diagram showing an image with observation distance D0, in the case where the size of a region of interest is not changed.

FIG. 4B is a diagram showing an image with observation distance D1, in the case where the size of a region of interest is not changed.

FIG. 4C is a diagram showing an image with observation distance D2, in the case where the size of a region of interest is not changed.

FIG. 5A is a diagram showing an image with observation distance D0, in the case where the size of a region of interest is changed.

FIG. 5B is a diagram showing an image with observation distance D1, in the case where the size of a region of interest is changed.

FIG. 5C is a diagram showing an image with observation distance D2, in the case where the size of a region of interest is changed.

FIG. 6 is a flowchart showing another method of calculating an exponent in the fluoroscopy apparatus according to the first embodiment of the present invention.

FIG. 7 is a diagram showing an example of a concentration conversion table provided in an image-combining unit of the fluoroscopy apparatus in FIG. 1.

FIG. 8 is a flowchart of image processing in the image processing unit in FIG. 1.

FIG. 9A is a graph showing the relationship between the luminance value of a corrected fluorescence image and the observation distance.

FIG. 9B is a graph showing, as a reference example, the relationship between the luminance value of a corrected fluorescence image and the observation distance.

FIG. 10 is a graph comparing the deviation of luminance values of a fluorescence image subjected to power arithmetic processing and the deviation of luminance values of a fluorescence image without power arithmetic processing.

FIG. 11 is a block diagram showing, in outline, the configuration of a fluoroscopy apparatus according to a first modification of the first embodiment of the present invention.

FIG. 12 is a flowchart of image processing in an image processing unit of a fluoroscopy apparatus according to a second modification of the first embodiment of the present invention.

FIG. 13 is a graph showing the relationship between the luminance value in a fluoroscopy apparatus according to a second modification of the first embodiment of the present invention and the amount of fluorescent agent present.

FIG. 14 is a graph showing the relationship between the luminance value, as a reference example, in the fluoroscopy apparatus in FIG. 13 and the amount of a fluorescent agent present.

FIG. 15 is a flowchart of image processing in an image processing unit of a fluoroscopy apparatus according to a third modification of the first embodiment of the present invention.

FIG. 16 is a diagram showing a state in which simultaneous observation of two identical standard specimens positioned at different observation distances is performed with a fluoroscopy apparatus according to a fifth modification of the first embodiment of the present invention.

FIG. 17A is a diagram showing the relationship between the luminance value of a fluorescence image obtained by the fluoroscopy apparatus according to the fifth modification of the first embodiment of the present invention and the observation distance.

FIG. 17B is a diagram showing the relationship between the luminance value of a reference image obtained by the

fluoroscopy apparatus according to the fifth modification of the first embodiment of the present invention and the observation distance.

FIG. 18 is a diagram showing a state in which simultaneous observation of two regions of interest in a standard specimen at different observation distances is performed with a fluoroscopy apparatus according to an eighth modification of the first embodiment of the present invention.

FIG. 19 is a diagram showing a state in which simultaneous observation of three or more regions of interest in a standard specimen at different observation distances is performed with a fluoroscopy apparatus according to a ninth modification of the first embodiment of the present invention.

FIG. 20 is a diagram showing a state in which simultaneous observation of regions of interest, including a continuous change in distance, in a standard specimen is performed with a fluoroscopy apparatus according to a tenth modification of the first embodiment of the present invention.

FIG. 21 is a diagram showing a standard deviation of FL/RL^a in a region of interest at every correction factor.

FIG. 22 is a block diagram showing, in outline, the configuration of a fluoroscopy apparatus according to a second embodiment of the present invention.

FIG. 23 is a diagram showing an example of a gain conversion table provided in a fluorescence-image normalization portion of the fluoroscopy apparatus in FIG. 22.

FIG. 24 is a flowchart of image processing in the image processing unit in FIG. 22.

FIG. 25 is a block diagram showing, in outline, the configuration of a fluoroscopy apparatus according to a third embodiment of the present invention.

FIG. 26 is a diagram showing an example of an excitation-light intensity conversion table provided in a fluorescence-image normalization portion of the fluoroscopy apparatus in FIG. 25.

FIG. 27 is a flowchart of image processing in the image processing unit in FIG. 25.

DESCRIPTION OF EMBODIMENTS

First Embodiment

A fluoroscopy system, a fluoroscopy apparatus, and a fluorescence-image processing method according to a first embodiment of the present invention will be described below with reference to the drawings.

As shown in FIG. 1, a fluoroscopy system 150 according to this embodiment is provided with a fluoroscopy apparatus 101 and a calibration device 102 that is combined with the fluoroscopy apparatus 101. The fluoroscopy apparatus 101 is an endoscope apparatus and is provided with an elongated insertion portion 2 that is inserted inside a body cavity, an illumination unit (illumination portion) 20 that includes a light source 10 that emits illumination light from an end 2a of the insertion portion 2, an image-acquisition unit 30 that is disposed in the insertion portion 2 and acquires image information of an observation target site X, which is the subject, an image processing unit 50 that performs arithmetic processing of the image information acquired by the image-acquisition unit 30, and a monitor 4 that displays the images etc. that are processed by the image processing unit 50.

The light source 10 is provided with a xenon lamp 12 that emits illumination light, a filter 14 that extracts the white light (illumination light) containing the excitation light from the illumination light emitted from the xenon lamp 12, and a coupling lens 16 that focuses the white light containing the excitation light extracted by the filter 14. The filter 14

11

extracts, for example, the white light containing the excitation light in a wavelength band between 400 and 750 nm.

The illumination unit **20** is provided with a light guide fiber **22** that is disposed along a longitudinal direction of the insertion portion **2** over nearly the entire length thereof and that guides the white light containing the excitation light focused by a coupling lens **16** to the end **2a** of the insertion portion **2**, and a spreading lens **24** that is disposed on the end **2a** of the insertion portion **2** and that spreads the white light containing the excitation light guided by the light guide fiber **22** to irradiate the observation target site X.

The image-acquisition unit **30** is provided with an objective lens **32** that collects return light returning from the observation target site X irradiated with the white light containing the excitation light by the illumination unit **20** and a dichroic mirror **34** that reflects light of the excitation wavelength or higher (the excitation light and fluorescence) in the return light collected by the objective lens **32**, and that transmits white light having a wavelength shorter than the excitation wavelength. The objective lens **32** and the spreading lens **24** are arranged side-by-side on the end **2a** of the insertion portion **2**.

This image-acquisition unit **30** is provided with an excitation-light cut filter **36** that blocks the excitation light in the excitation light and fluorescence reflected by the dichroic mirror **34** and that transmits only the fluorescence (for example, near-infrared fluorescence), two focusing lenses **38** that respectively focus the fluorescence transmitted through this excitation-light cut filter **36** and the white light transmitted through the dichroic mirror **34**, a fluorescence-imaging unit **42** that images the fluorescence focused by the focusing lenses **38** to obtain the fluorescence image information, and a white-light-imaging unit (return-light imaging unit) **44** that images the white light focused by the focusing lenses **38** to obtain the reference image information.

The excitation-light cut filter **36** only transmits, for example, fluorescence in the wavelength band between 765 and 850 nm.

The fluorescence-imaging unit **42** is, for example, a high-sensitivity monochrome CCD for fluorescence. The white-light-imaging unit **44** is, for example, a color CCD for white light and is provided with a mosaic filter (not shown).

The image processing unit **50** is provided with a fluorescence exposure-time adjusting portion (image-acquisition condition adjusting portion) **54** that adjusts the exposure time (image acquisition condition) of the fluorescence-imaging unit **42** and a fluorescence-image generating unit **52** that generates a two-dimensional fluorescence image on the basis of the fluorescence image information acquired by the fluorescence-imaging unit **42**, a white-light exposure-time adjusting unit (image-acquisition condition adjusting portion) **58** that adjusts the exposure time (image acquisition condition) of the white-light-imaging unit **44** and a reference-image generating unit **56** that generates a two-dimensional reference image on the basis of the reference image information acquired by the white-light-imaging unit **44**, and an image-correction unit **60** that corrects the fluorescence image generated by the fluorescence-image generating unit **52** using the reference image generated by the reference-image generating unit **56**.

The fluorescence exposure-time adjusting portion **54** adjusts the exposure time of the fluorescence-imaging unit **42** on the basis of the luminance values of the fluorescence image generated by the fluorescence-image generating unit **52**.

Similarly, the white-light exposure-time adjusting unit **58** adjusts the exposure time of the white-light-imaging unit **44**

12

on the basis of the luminance values of the reference image generated by the reference-image generating unit **56**.

The image-correction unit **60** is provided with a fluorescence-image normalization portion **62** that normalizes the luminance of the fluorescence image generated by the fluorescence-image generating unit **52** and a fluorescence-image preprocessing section **64** that performs arithmetic processing on the fluorescence image whose luminance is normalized; a reference-image normalization portion **66** that normalizes the luminance of the reference image obtained by the reference-image generating unit **56** and a reference-image preprocessing section **68** that performs arithmetic processing on the reference image whose luminance is normalized; and a division processing unit **72** that obtains a corrected fluorescence image K by dividing the correction fluorescence image obtained by the fluorescence-image preprocessing section **64** by the correction reference image obtained by the reference-image preprocessing section **68**.

The fluorescence-image normalization portion **62** reads out the luminance value of the fluorescence image from the fluorescence-image generating unit **52** and divides it by the exposure time of the fluorescence-imaging unit **42** set by the fluorescence exposure-time adjusting portion **54**.

The fluorescence-image preprocessing section **64** obtains the correction fluorescence image by raising the normalized luminance value of the fluorescence image to the power of the reciprocal $1/\alpha$ (or $-1/\alpha$) of a first exponent α that is obtained by a power approximation of a distance characteristic of luminance versus observation distance D_n for the fluorescence image, which is obtained by the fluorescence-imaging unit **42** by radiating the excitation light of a prescribed intensity onto the observation target site X and which is normalized by the fluorescence-image normalization portion **62**. Specifically, the power computation shown below is performed:

$$FL_{after} = A \times FL_{before}^x \quad (1)$$

Here, FL_{after} is a luminance value of the correction fluorescence image, FL_{before} is a luminance value of the fluorescence image, x is $1/\alpha$ or $-1/\alpha$, α is a first exponent, and A is a constant.

By performing this power computation, the correction fluorescence image whose luminance is proportional to (with $-1/\alpha$, inversely proportional to) the variation of the distance is obtained.

Similarly, the reference-image normalization portion **66** reads out the luminance information of the reference image from the reference-image generating unit **56** and divides it by the exposure time of the white-light-imaging unit **44** set by the white-light exposure-time adjusting unit **58**.

In addition, the reference-image preprocessing section **68** obtains the correction reference image by raising the normalized luminance value of the reference image to the power of reciprocal $1/\beta$ (or $-1/\beta$) of a second exponent β that is obtained by a power approximation of a distance characteristic of luminance versus observation distance D_n for the reference image, which is obtained by the white-light-imaging unit **44** by radiating the white light of a prescribed intensity onto the observation target site X and which is normalized by the reference-image normalization portion **66**. Specifically, the power computation shown below is performed:

$$RL_{after} = B \times RL_{before}^y \quad (2)$$

Here RL_{after} is a luminance value of the correction reference image, RL_{before} is a luminance value of the reference image, y is $1/\beta$ or $-1/\beta$, β is a second exponent, and B is a constant.

By performing this power computation, the correction reference image whose luminance is proportional to (with $-1/\beta$, inversely proportional to) the variation of the distance is obtained.

In this case, based on a determination made prior to the fluorescence observation, the first exponent α and the second exponent β are decided, as described below, by, as shown in FIG. 2, disposing a standard specimen **81** so as to oppose the end **2a** of the insertion portion **2**, and using the calibration device **102**.

The calibration device **102** is provided with a translation stage (observation-state setting mechanism) **92** that changes the distance D_n (hereinafter referred to as “observation distance”) between the end **2a** of the insertion portion **2** and the standard specimen **81**, a stage controller **94** that controls the position of the translation stage **92**, a distance-information detector **96** that detects the distance information of the observation distance D_n , and a dependency-constant determining unit (exponent calculating unit) **98** that calculates the first exponent α and the second exponent β .

The dependency-constant determining unit **98** calculates the first exponent α and the second exponent β on the basis of the normalized fluorescence image and reference image sent from the fluorescence-image normalization portion **62** and the reference-image normalization portion **66**, respectively, and on the basis of the distance information detected by the distance-information detector **96**.

As the standard specimen **81**, for example, one having an optical characteristic close to that of a living body, such as tissue from a pig large intestine, injected with fluorescent dye is desirable.

The method of calculating the first exponent α and the second exponent β in the dependency-constant determining unit **98** will be described below with reference to a flowchart in FIG. 3.

The observation distance D_n is first set by operating the stage controller **94** (step SC1), and the observation distance D_n at this time is detected by the distance-information detector **96** and sent to the dependency-constant determining unit **98**. In this state, the white light containing the excitation light is radiated onto the standard specimen **81** from the illumination unit **20**. Then, the fluorescence and the white light are captured respectively with the fluorescence-imaging unit **42** and the white-light-imaging unit **44**, and the fluorescence image and the reference image are obtained by the fluorescence-image generating unit **52** and the reference-image generating unit **56** (step SC2).

Next, the average values of the luminance values of regions that are determined in advance (hereinafter referred to as “regions of interest”) of the acquired fluorescence image and reference image are calculated (step SC3).

The method of obtaining the luminance values is explained with the following reference example as an illustration.

For example, as shown in FIG. 2, the illumination light is radiated onto the standard specimen **81** while changing the observation distance D_n to D_0 , D_1 , and D_2 ($D_0 < D_1 < D_2$) to obtain the fluorescence images such as those shown in FIGS. 4A to 4C and FIGS. 5A to 5C. In FIG. 2, reference sign **83** is a field of view of the fluorescence-imaging unit **42** and reference sign **85** is a region of interest.

If the fluorescence intensity in the standard specimen **81** is constant, in other words, for example, if the surface of the standard specimen **81**, which is the subject, is substantially

flat, as shown in FIGS. 4A to 4C, the luminance value is calculated by making the size of the region of interest **85** constant regardless of the observation distance D_n . On the other hand, if the fluorescence intensity in the standard specimen **81** is not constant, in other word, for example, if there are irregularities on the surface of the standard specimen **81** and if there are nonuniformities in the fluorescence distribution in the standard specimen **81**, as shown in FIGS. 5A to 5C, the luminance value is calculated by changing the size of the region of interest **85** in accordance with the observation distance D_n . By changing the size of the region of interest **85**, it is possible to obtain the luminance value of the same site even when the observation distance D_n is changed.

Next, the average values of the luminance values in the regions of interest, which are calculated from the fluorescence image and reference image, are divided by the exposure time and normalized by the fluorescence-image normalization portion **62** and the reference-image normalization portion **66** (step SC4), respectively, and thereafter, they are sent to the dependency-constant determining unit **98**, and the luminance values are plotted in association with the distance information (step SC5).

The stage controller **94** repeats the above-described steps SC1 to SC6 multiple times for a predetermined number of times a (a is at least two or more) (step SC6). For example, the observation distance D_n is changed to D_0 and D_1 , for example, a regression curve is obtained by a power approximation of the obtained distance characteristics, in other words, by performing regression to power functions D^α and D^β (step SC7), and thereby, the first exponent α and the second exponent β that indicate the dependencies on the observation distance D_n are calculated (step SC8). The results of the determination of the first exponent α and the second exponent β from the regression curve, as the reference examples, are shown in FIGS. 17A and 17B. In FIGS. 17A and 17B, the vertical axis indicates the luminance value in the fluorescence image or the reference image and the horizontal axis indicates the observation distance D_n .

By doing so, it is possible to determine the observation distance D_n and corresponding accurate exponents for the fluorescence image and the reference image with the dependency-constant determining unit **98**. The first exponent α and the second exponent β determined by the dependency-constant determining unit **98** are sent to the fluorescence-image preprocessing section **64** and the reference-image preprocessing section **66**, respectively.

In this embodiment, the distance-information detector **96** may be omitted, and distance information of the observation distance D_n may be input to the dependency-constant determining unit **98** manually.

In addition, in this embodiment, although the average values of the luminance values of the regions of interest in the fluorescence image and the reference image are calculated before the normalization (see step SC3 in FIG. 3), and thereafter, the average values are normalized by treating them as the luminance values and dividing them by the exposure time (see SC4 in FIG. 3), instead of this, as shown in the flowchart in FIG. 6, for example, the normalization may be performed by dividing the luminance of the whole fluorescence image and the luminance of the whole reference image by the exposure time, respectively (step SC3'), and thereafter, the average values of the normalized luminance values of the regions of interest in the fluorescence image and the reference image may be calculated (step SC4').

In addition, the image processing unit **50** is provided with an image-combining unit **74** that generates an image by combining the reference image S generated by the reference-

image generating unit 56 and the corrected fluorescence image K generated by an image-correction unit 75. The image-combining unit 74 combines the corrected fluorescence image K obtained by the division processing unit 72 and the reference image S generated by the reference-image generating unit 56 such that the combined images are arranged in parallel and simultaneously displayed on the monitor 4. In addition, as shown in FIG. 7, the image-combining unit 74 has a concentration conversion table 87 in which the luminance values of the corrected fluorescence image K and the amount of fluorescent agent present (in other words, the concentration of fluorescent agent) are associated with each other, which allows the fluorescence concentration in a specific region to be displayed on the monitor 4.

The operation of the thus-configured fluoroscopy apparatus 101 and fluorescence-image processing method according to this embodiment will be described.

In order to perform observation of, for example, an observation target site X in a body cavity of a living body using the fluoroscopy apparatus 101 according to this embodiment, the insertion portion 2 is inserted into the body cavity, and the end 2a is directed so as to oppose the observation target site X.

In this state, the illumination unit 20 is operated, and the white light containing the excitation light, which is emitted from the xenon lamp 12 and extracted by the filter 14, is focused by the coupling lens 16 so as to enter the light guide fiber 22. The white light containing the excitation light that has entered the light guide fiber 22 is guided to the end 2a of the insertion portion 2, is spread by the spreading lens 24, and is radiated onto the observation target site X.

In the observation target site X, the fluorescent agent contained therein is excited by the excitation light, emitting fluorescence, and the white light is reflected at the surface of the observation target site X. The fluorescence and the return light from the white light are collected by the objective lens 32 of the insertion portion 2 and are split into different wavelengths by the dichroic mirror 34.

At the dichroic mirror 34, the light of the excitation wavelength or higher, in other words, the excitation light, and fluorescence are reflected, and the white light having a shorter wavelength than the excitation wavelength is transmitted.

The excitation light among the excitation light and fluorescence reflected at the dichroic mirror 34 is removed by the excitation-light cut filter 36, and only the fluorescence is focused by the focusing lens 38. The fluorescence is captured by the fluorescence-imaging unit 42 and is obtained as the fluorescence image information.

In addition, the white light transmitted through the dichroic mirror 34 is focused by the focusing lens 38, is captured by the white-light-imaging unit 44, and is obtained as the reference image information.

Either fluorescence image information or the reference image information can be obtained before the other, or both can be obtained simultaneously.

The fluorescence image information obtained by the fluorescence-imaging unit 42 and the reference image information obtained by the white-light-imaging unit 44 are individually input to the image processing unit 50 and subjected to image processing. The image processing in the image processing unit 50 will be described below with reference to a flowchart in FIG. 8.

In the image processing unit 50, the fluorescence image information is input to the fluorescence-image generating unit 52, where a two-dimensional fluorescence image is generated. In this case, the exposure time of the fluorescence-imaging unit 42 is set by the fluorescence exposure-time adjusting portion 54 on the basis of the luminance value of the

fluorescence image generated by the fluorescence-image generating unit 52 (step SF1). By doing so, a fluorescence image having suitable brightness is obtained by the fluorescence-image generating unit 52 regardless of the luminance of the fluorescence emitted from the observation target site X (step SF2).

Similarly, the reference image information is input to the reference-image generating unit 56, where a two-dimensional reference image is generated. In this case, the exposure time of the white-light-imaging unit 44 is adjusted by the white-light exposure-time adjusting unit 58 on the basis of the luminance value of the reference image generated by the reference-image generating unit 56 (step SR1). By doing so, a reference image having suitable brightness is obtained by the reference-image generating unit 56 regardless of the luminance of the white light returned from the observation target site X (step SR2).

The fluorescence image generated by the fluorescence-image generating unit 52 and the reference image generated by the reference-image generating unit 56 are individually sent to the image-correction unit 60.

In the image-correction unit 60, first, the fluorescence-image normalization portion 62 divides the luminance value of the fluorescence image by the exposure time of the fluorescence-imaging unit 42 (step SF3). By doing so, the differences in the exposure time in the fluorescence image are normalized, and the fluorescence image is standardized at luminance value per unit time. In addition, the reference-image normalization portion 66 divides the luminance value of the reference image by the exposure time of the white-light-imaging unit 44 (step SR3). By doing so, the differences in the exposure time in the reference image are normalized, and the reference image is standardized at luminance value per unit time.

The fluorescence image whose luminance has been normalized by the fluorescence-image normalization portion 62 is sent to the fluorescence-image preprocessing section 64, and the reference image whose luminance has been normalized by the reference-image normalization portion 66 is sent to the reference-image preprocessing section 68.

Next, in the fluorescence-image preprocessing section 64, in accordance with the above-mentioned correction arithmetic expression (1), the luminance value of each pixel in the fluorescence image is raised to the power of the reciprocal $1/\alpha$ of the first exponent α (step SF4). By doing so, information related to the power of the distance is cancelled, and a correction fluorescence image in which the luminance is proportional to the variation of the distance is obtained. In addition, in the reference-image preprocessing section 68, in accordance with the above-mentioned correction arithmetic expression (2), the luminance value of each pixel in the reference image is raised to the power of the reciprocal $1/\beta$ of the second exponent β (step SR4). By doing so, information related to the power of the distance is cancelled, and a correction reference image in which the luminance is proportional to the variation of the distance is obtained.

The correction fluorescence image and the correction reference image are individually sent to the division processing unit 72, where the correction fluorescence image is divided by the correction reference image (step SFR5). Since the correction fluorescence image and the correction reference image are related to each other such that the luminance is proportional to the variations of the distances by performing the above-mentioned power arithmetic processing, as shown in FIG. 9A, by dividing the correction fluorescence image by the correction reference image, it is possible to obtain a corrected fluorescence image K having quantitiveness, in which the

dependencies on distance are cancelled, and the correction is achieved with a high accuracy.

The corrected fluorescence image K and the correction reference image obtained in the division processing unit 72 are sent to the image-combining unit 74. In the image-combining unit 74, the corrected fluorescence image K and the reference image S are combined and displayed on the monitor 4 simultaneously, and on the basis of the concentration conversion table 87, the fluorescence concentration in a specific region is displayed on the monitor 4.

As described above, according to the fluoroscopy apparatus 101 and fluorescence-image processing method of this embodiment, by subjecting the fluorescence image to the correction processing after processing the information related to the power of the distance contained in the fluorescence image and the reference image, it is possible to perform observation by obtaining the corrected fluorescence image K having high quantitiveness, in which the dependencies on distance of the fluorescence image and the reference image are cancelled. By doing so, it is possible to diagnose a lesion accurately from the luminance values of the corrected fluorescence image K.

As a reference example, the relationship between the luminance value of the fluorescence image and the observation distance D_n when the fluorescence image is divided by the reference image without performing power arithmetic processing is shown in FIG. 9B. Since each of the fluorescence image and the reference image that is not subjected to power arithmetic processing contains the information related to the power of the distance, the dependencies on the distance cannot be completely cancelled by a simple division of the fluorescence image by the reference image, and the influence of distance remains in the divided fluorescence image. FIG. 10 shows the relationship between the observation distance D_n and the deviations from the average values of the luminance values of the fluorescence image with/without the power computation. In FIG. 10, the vertical axis indicates the deviation (%) from the average value of the luminance value and the horizontal axis indicates the observation distance D_n .

In addition, in this embodiment, although a correction factor for the fluorescence-image preprocessing section 64 is illustrated as $x=1/\alpha$ and a correction factor for the reference-image preprocessing section 68 is illustrated as $y=1/\beta$, correction factors obtained by respectively multiplying x and y by a constant k may be used. Similar effects can also be achieved in this case.

In addition, if α or β is chosen for the value of the constant k , it is possible to make the correction factor of either the fluorescence-image preprocessing section 64 or the reference-image preprocessing section 68 equal to unity, thereby reducing the amount of calculation.

This embodiment can be modified as follows.

For example, as a first modification, as shown in FIG. 11, the configuration may include the fluoroscopy apparatus 100 only and may omit the calibration device. In such a case, the preset correction factor x is stored in the fluorescence-image preprocessing section 64, and a preset correction factor y is stored in the reference-image preprocessing section 66.

In a second modification, for example, as shown in a flowchart in FIG. 12, in the image-correction unit 60, a postprocessing section (not shown) may be provided between the division processing unit 72 and the image-combining unit 74, and the postprocessing section may further raise the luminance value of each pixel in the corrected fluorescence image K obtained by the division processing unit 72 to the power of the first exponent α (step SFR6). By doing so, as shown in FIG. 13, it is possible to reduce the dependency on the dis-

tance by using the postprocessing section while maintaining the proportional relationship between the luminance value of the corrected fluorescence image K and the amount of fluorescent agent present (i.e., the concentration of fluorescent agent). As a reference example, FIG. 14 shows the relationship between the luminance value of the corrected fluorescence image K and the concentration of fluorescent agent when the luminance value is not raised to the power of the first exponent α by the postprocessing section.

In this embodiment, although the image-correction unit 60 is provided with the fluorescence-image preprocessing section 64, in a third modification, for example, the fluorescence-image preprocessing section 64 may be omitted, and the reference-image preprocessing section 68 may obtain the correction reference image by raising the luminance value of the reference image to the power of a third exponent α/β (or α/β) that is obtained by dividing the first exponent α by the second exponent β .

In this case, as shown in a flowchart in FIG. 15, the fluorescence image normalized by the fluorescence-image normalization portion 62 may be sent to the division processing unit 72, and the power computation as described below may be performed by the reference-image preprocessing section 68 (step SR4'):

$$RL_{after} = B \times RL_{before}^z \quad (3)$$

Here, RL_{after} is a luminance value of the correction reference image, RL_{before} is a luminance value of the reference image, z is a third exponent (α/β or $-\alpha/\beta$), α is a first exponent, β is a second exponent, and B is a constant.

By doing so, in the image-correction unit 60, it is sufficient to perform the power computation only once to correct the influence of the distance with high precision, and it is possible to obtain the corrected fluorescence image K in which the luminance value and the amount of the fluorescent agent present are in a directly proportional relationship.

In this embodiment, although the image-correction unit 60 is provided with the reference-image preprocessing section 66, in a fourth modification, for example, the reference-image preprocessing section 66 may be omitted, and the fluorescence-image preprocessing section 64 may obtain the correction fluorescence image by raising the luminance value of the fluorescence image to the power of a fourth exponent β/α (or $-\beta/\alpha$) that is obtained by dividing the second exponent β by the first exponent α , that is, the reciprocal of the third exponent α/β (or $-\alpha/\beta$).

In this case, the reference image normalized by the reference-image normalization portion 66 may be sent to the division processing unit 72, and the power computation as described below may be performed by the fluorescence-image preprocessing section 64:

$$FL_{after} = A \times FL_{before}^{z'} \quad (4)$$

Here, FL_{after} is a luminance value of the correction fluorescence image, FL_{before} is a luminance value of the fluorescence image, z' is a fourth exponent β/α (or $-\beta/\alpha$), α is a first exponent, β is a second exponent, and A is a constant.

By doing so, in the image-correction unit 60, it is sufficient to perform the power computation only once to correct the influence of the distance with high precision.

In the third modification, although the reference-image preprocessing section 68 obtains the correction reference image by raising the luminance value of the reference image to the power of the third exponent α/β (or $-\alpha/\beta$), serving as the correction factor z , in a fifth modification, instead of the correction factor z , the correction factor (second correction factor) a , which is defined in the following method may be

used in a dependency-constant determining unit (correction-factor calculating unit) (not shown).

As shown in FIG. 16, when two identical standard specimens **81** are positioned at different observation distances **D0** and **D1** within the range of the field of view of the fluorescence-imaging unit **42** and the white-light-imaging unit **44** and observed simultaneously, the correction factor *a* is set such that the luminance value obtained from the region of interest **85** of the corrected fluorescence image positioned at the observation distance **D0** substantially matches the luminance value obtained from the region of interest **85** of the corrected fluorescence image positioned at the observation distance **D1**.

Specifically, the correction factor *a* that is obtained in the following arithmetic expression is calculated, in other words, the correction factor *a* is calculated such that the ratio of the fluorescence image to the correction reference image in which the luminance value of the reference image of the standard specimen **81** positioned at the observation distance **D0** is raised to the power of the correction factor *a* substantially matches the ratio of the fluorescence image to the correction reference image in which the luminance value of the reference image of the standard specimen **81** positioned at the observation distance **D1** is raised to the power of the correction factor *a*:

$$FL(D0)/RL(D0)^a = FL(D1)/RL(D1)^a \quad (5)$$

$$a = \log(FL(D1)/FL(D0)) / \log(RL(D1)/RL(D0)) \quad (6)$$

Here, $FL(D0)$ is a luminance value of the fluorescence image at the observation distance **D0**, $RL(D0)$ is a luminance value of the reference image at the observation distance **D0**, $FL(D1)$ is a luminance value of the fluorescence image at the observation distance **D1**, and $RL(D1)$ is a luminance value of the reference image at the observation distance **D1**.

The reference-image preprocessing section **68** obtains the correction reference image of the observation target site **X** in a body cavity of a living body in accordance with the following arithmetic expression and sends it to the division processing unit **72**:

$$RL_{after} = B \times RL_{before}^a \quad (7)$$

According to expressions (5) and (6), the correction factor *a* is calculated such that the luminance values at two locations at different observation distances (**D0** and **D1**) in the corrected fluorescence image **K** match each other. On the other hand, as shown in FIGS. 17(A) and 17(B), although the distance dependencies of the luminance value of the fluorescence image and of the luminance value of the reference image differ in the exponent, that is, the power of the distance, both are in a substantially inversely proportional relationship with respect to the power of the distance. Therefore, the values of the correction factor *a* decided at two locations that differ in the observation distances become close to the third exponent α/β , and it is possible to reduce the difference in the distance dependencies even when correction using the correction factor *a* is performed on an image with an observation distance other than the observation distances **D0** and **D1**.

If the observation distances **D0** and **D1** are close to each other, because the differences between the luminance values of the fluorescence images and the luminance values of the reference images at respective distances are small and errors tend to occur, it is preferred that the difference between the values of the observation distances **D0** and **D1** be as large as possible.

It is not required to obtain a plurality of images by changing the observation distance **Dn** to obtain exponents from power

approximations, and even when the observation distances **D0** and **D1** are unknown, it is possible to calculate a correction factor *a* and to set the correction factor *a* easily.

In the fourth modification, although the fluorescence-image preprocessing section **64** obtains the correction fluorescence image by raising the luminance value of the fluorescence image to the power of the reciprocal of the third exponent β/α (or $-\beta/\alpha$), in a sixth modification, the correction may be performed using the reciprocal (first correction factor) $1/a$ of the correction factor *a* calculated in the fifth modification.

Specifically:

$$FL_{after} = A \times FL_{before}^{(1/a)} \quad (8)$$

With this configuration, effects similar to those in the fifth modification can be achieved.

In the fourth modification, although the correction factor *a* is set as a correction value for the reference-image preprocessing section **64**, such that the luminance values of the corrected fluorescence image in two identical standard specimens **81** at different observation distances **Dn** substantially match, in a seventh modification, correction factors (first correction factor and second correction factor) *b* and *c* obtained in accordance with the following arithmetic expressions may be set as the correction factors for the fluorescence-image preprocessing section **64** and the reference-image preprocessing section **68**, respectively:

$$FL(D0)^b / RL(D0)^c = FL(D1)^c / RL(D1)^c \quad (9)$$

$$c/b = \log(FL(D1)/FL(D0)) / \log(RL(D1)/RL(D0)) \quad (10)$$

In expression (10), although the ratio of *b* and *c* can be derived, numerical values cannot be decided. Thus, the value of *c* can be decided in accordance with expression (10) by arbitrarily setting the value of *b* (for example 2). Instead of this, after the value of *c* is set arbitrarily, the value of *b* may be decided in accordance with expression (10).

The decided correction factor *b* is set in the fluorescence-image preprocessing section **64**, and the fluorescence-image preprocessing section **64** performs the following computation:

$$FL_{after} = A \times FL_{before}^b \quad (11)$$

The decided correction factor *c* is set in the reference-image preprocessing section **68**, and the reference-image preprocessing section **68** performs the following computation:

$$RL_{after} = B \times RL_{before}^c \quad (12)$$

The value obtained by dividing the correction factor *c* by the correction factor *b* is equal to the correction factor *a* calculated in the fourth modification, and it also has a value close to that of the third exponent α/β . This modification also achieves effects equivalent to those in the fourth modification.

In the fifth to seventh modifications, although two identical standard specimens **81** are positioned at different observation distances **D0** and **D1**, and the correction factors *a* are calculated from the luminance values obtained from the respective regions of interest **85**, in an eighth modification, as shown in FIG. 18, the standard specimen **81** may be placed at an angle within the ranges of the fields of view of the fluorescence-imaging unit **42** and the white-light-imaging unit **44**, and the correction factors *a* may be calculated from the luminance values obtained from two regions of interest **85** located at different observation distances **Dn** on one standard specimen **81**.

In this case, as in this embodiment, the correction factor *a*, and the correction factors *b* and *c* may be calculated such that the luminance value obtained in the region of interest **85** in the

21

corrected fluorescence image at the observation distance D0 substantially matches the luminance value obtained in the region of interest 85 in the corrected fluorescence image at the observation distance D1. By doing so, it is possible to set the correction factors a, b, and c easily by using only one standard specimen 81.

In the fifth modification, although the correction factor a is set by the luminance values obtained from two regions of interest 85 located at different observation distances Dn, in a ninth modification, as shown in FIG. 19, the correction factor a may be calculated from the luminance values of two regions of interest 85 having observation distances Dn that are close to each other among the luminance values obtained from three or more regions of interest 85 in the standard specimen 81 placed at an angle within the ranges of the fields of view of the fluorescence-imaging unit 42 and the white-light-imaging unit 44.

For example, a correction factor a01 in which the luminance value obtained from the region of interest 85 at the observation distance D0 substantially matches the luminance value obtained from the region of interest 85 at the observation distance D1 and a correction factor a02 in which the luminance value obtained from the region of interest 85 at the observation distance D1 substantially matches the luminance value obtained from the region of interest 85 at the observation distance D2 may be calculated, and the correction factor a may be derived from the average values $(a=(a01+a02)/2)$ of each of the correction factors a01 and a02. By doing so, it is possible to reduce the errors caused in the correction factors a on the basis of the luminance values of a plurality of regions of interest 85.

In a tenth modification, as shown in FIG. 20, with the standard specimen 81 placed at an angle within the ranges of the fields of view of the fluorescence-imaging unit 42 and the white-light-imaging unit 44, a region including a continuous distance change, for example, from the observation distance D0 to the observation distance D1, may be set as the region of interest 85, the correction factor a may be varied from 1 in increments of 0.05 to calculate FL/RL^a for every pixel in the region of interest 85, and, as shown in FIG. 21, the standard deviation σ of FL/RL^a in the region of interest 85 for every correction factor a may be calculated, and thereby, the correction factor a that yields the smallest standard deviation σ may be set. By doing so, the errors caused in the correction factor a can be reduced.

Second Embodiment

Next, a fluoroscopy apparatus and fluorescence-image processing method according to a second embodiment of the present invention will be described.

The fluoroscopy apparatus 200 according to this embodiment differs from the first embodiment in that, as shown in FIG. 22, the image processing unit 250 is provided with, instead of the fluorescence exposure-time adjusting portion 54, a fluorescence-gain-value adjusting portion (image-acquisition condition adjusting portion) 254 that adjusts a gain value (image acquisition condition, gain factor) that amplifies the fluorescence image information acquired by the fluorescence-imaging unit 42.

In the following, parts having the same configuration as those in the fluoroscopy apparatuses 100 and 101 according to the first embodiment will be assigned the same reference signs, and a description thereof will be omitted.

The fluorescence-gain-value adjusting portion 254 adjusts the gain value of the fluorescence-imaging unit 42 on the

22

basis of the luminance value of the fluorescence image generated by the fluorescence-image generating unit 52.

The gain value of the fluorescence-imaging unit 42 that is set by the fluorescence-gain-value adjusting portion 254 is input to the fluorescence-image normalization portion 62. In addition, the fluorescence-image normalization portion 62 is provided with a gain-factor conversion table 287, like that shown in FIG. 23, in which gain values and gain multiplication factors are associated with each other.

With the thus-configured fluoroscopy apparatus 200, as shown in a flowchart in FIG. 24, the gain value of the fluorescence-imaging unit 42 is set by the fluorescence-gain-value adjusting portion 254 on the basis of the luminance value of the fluorescence image generated by the fluorescence-image generating unit 52 (step SG1). By doing so, a fluorescence image having suitable brightness is obtained by the fluorescence-image generating unit 52 regardless of the incident light intensity of the fluorescence generated at the observation target site X (step SG2).

In the fluorescence-image normalization portion 62, the luminance value of the fluorescence image read out from the fluorescence-image generating unit 52 is divided by the gain multiplication factor that corresponds to the gain value at the time of acquisition of the fluorescence image by the fluorescence-imaging unit 42 (step SG3). By doing so, the influence of the gain value in the fluorescence image is normalized, and the fluorescence image can be standardized at a certain luminance value per multiplication value.

Third Embodiment

Next, a fluoroscopy apparatus and a fluorescence-image processing method according to a third embodiment of the present invention will be described.

The fluoroscopy apparatus 300 according to this embodiment differs from the first embodiment in that, as shown in FIG. 25, the light source 310 is further provided with a semiconductor laser 312, and the image processing unit 350 is provided with, instead of the fluorescence exposure-time adjusting portion 54 and the white-light exposure-time adjusting unit 58, an excitation-light adjusting portion (image-acquisition condition adjusting portion) 354 that adjusts the light-adjustment level of the excitation light emitted from the illumination unit 20 and a white-light adjusting portion (image-acquisition condition adjusting portion) 358 that adjusts the light-adjustment level of the illumination light.

In the following, parts having the same configuration as those in the fluoroscopy apparatuses 100 and 101 according to the first embodiment will be assigned the same reference signs, and a description thereof will be omitted.

The light source 310 is provided with the xenon lamp 12, a xenon lamp controller 13, an infrared-cut filter 314 that blocks infrared light in the illumination light and transmits only the white light emitted from the xenon lamp 12, the semiconductor laser 312 that emits the excitation light in the wavelength band of 740 nm, a semiconductor laser controller 313, and a light source dichroic mirror 315 that transmits the white light transmitted through the infrared-cut filter 314 and that reflects the excitation light emitted from the semiconductor laser 312, thereby guiding the white light and the excitation light into the same optical path. The infrared-cut filter 314 transmits only, for example, the white light in the wavelength band between 400 and 680 nm. Reference sign 316A is a first coupling lens that focuses the white light transmitted through the infrared-cut filter 314, and reference sign 316B is a second coupling lens that focuses the white light and the

excitation light that are guided into the same optical path by the light-source dichroic mirror **315**.

The excitation-light adjusting portion **354** adjusts the light-adjustment level of the semiconductor laser **312** with the semiconductor laser controller **313** on the basis of the luminance value of the fluorescence image generated by the fluorescence-image generating unit **52**.

Similarly, the white-light adjusting portion **358** adjusts the light-adjustment level of the xenon lamp **12** with the xenon lamp controller **13** on the basis of the luminance value of the reference image generated by the reference-image generating unit **56**.

The light-adjustment level of the semiconductor laser controller **313** that is set by the excitation-light adjusting portion **354** is input to the fluorescence-image normalization portion **62**. The fluorescence-image normalization portion **62** is provided with an excitation-light intensity conversion table **387**, like that shown in FIG. **26**, in which the light-adjustment level and the excitation-light intensity are associated with each other.

Similarly, the light-adjustment level of the xenon lamp controller **13** that is set by the white-light adjusting portion **358** is input to the reference-image normalization portion **66**. The reference-image normalization portion **66** is provided with a white-light intensity conversion table (not shown) in which the light-adjustment level and the white-light intensity (illumination light intensity) are associated with each other. The excitation-light intensity and the white-light intensity may be decided by respective intensity ratios based on the minimum values.

With the thus-configured fluoroscopy apparatus **300**, the white light emitted from the xenon lamp **12**, transmitted through the infrared-cut filter **314**, and focused by the first coupling lens **316A** is transmitted through the light source dichroic mirror **315**, and the excitation light emitted from the semiconductor laser **312** is reflected at the light source dichroic mirror **315**, and both the white light and the excitation light are guided along the same optical path and are focused by a second coupling lens **316B** so as to enter the light guide fiber **22**.

In the image-correction unit **60**, as shown in a flowchart in FIG. **27**, the light-adjustment level of the semiconductor laser controller **313** is set by the excitation-light adjusting portion **354** on the basis of the luminance value of the fluorescence image generated by the fluorescence-image generating unit **52** (step SL1). By doing so, in the fluorescence-image generating unit **52**, a fluorescence image having suitable brightness is obtained by varying the intensity of the fluorescence generated at the observation target site X (step SL2).

Similarly, the light-adjustment level of the xenon lamp controller **13** is set by the white-light adjusting portion **358** on the basis of the luminance value of the reference image generated by the reference-image generating unit **56** (step SM1). By doing so, in the reference-image generating unit **56**, a reference image having suitable brightness is obtained by varying the intensity of the white light returning from the observation target site X (step SM2).

Then, the fluorescence-image normalization portion **62** performs division of the luminance value of the fluorescence image read out from the fluorescence-image generating unit **52** by the excitation-light intensity corresponding to the light-adjustment level of the semiconductor laser controller **313** (step SL3). By doing so, the influence of the light-adjustment level of the excitation light is normalized, and the fluorescence image can be standardized at a certain luminance value per unit of excitation-light intensity.

In addition, the reference-image normalization portion **66** divides the luminance value of the reference image read out from the reference-image generating unit **56** by the white-light intensity corresponding to the light-adjustment level of the xenon lamp controller **13** (step SM3). By doing so, the influence of the light-adjustment level of the illumination light is normalized, and the reference image can be standardized at a certain luminance value per unit of white-light intensity.

Although the embodiments of the present invention have been described above with reference to the drawings, the specific configurations are not limited to these embodiments, and design alterations and the like within a range that does not depart from the spirit of the present invention are encompassed. For example, the present invention is not limited to aspects that are employed in the above-described embodiments and modifications thereof; without particular limitation, it may also be applied to embodiments formed by appropriately combining these embodiments and modifications thereof.

In addition, each of the above-mentioned embodiments has been described in terms of examples where near-infrared fluorescence and white light are used. However, the present invention is not limited thereto and, for example, fluorescence having visible wavelengths may be used in place of the near-infrared fluorescence, or excitation light having visible wavelengths may be used in place of the white light. In addition, for example, in the fluorescence-image preprocessing section **64** and the reference-image preprocessing section **68**, the power computation may be performed after noise components in the fluorescence-imaging unit **42** and the white-light-imaging unit **44** have been subtracted. By doing so, the precision of the power computation can be improved.

REFERENCE SIGNS LIST

- 10, 310** light source
- 20** illumination unit (illumination portion)
- 42** fluorescence-imaging unit
- 44** white-light-imaging unit (return-light imaging unit)
- 54** fluorescence exposure-time adjusting portion (image-acquisition condition adjusting portion)
- 58** white-light exposure-time adjusting unit (image-acquisition condition adjusting portion)
- 60, 460** image-correction unit
- 92** translation stage (observation-state setting mechanism)
- 98** dependency-constant determining unit (exponent calculating unit, correction-factor calculating unit)
- 100, 101, 200, 300, 400** fluoroscopy apparatus
- 102** calibration device
- 150** fluoroscopy system
- 254** fluorescence-gain-value adjusting portion (image-acquisition condition adjusting portion)
- 354** excitation-light adjusting portion (image-acquisition condition adjusting portion)
- 358** white-light adjusting portion (image-acquisition condition adjusting portion)

What is claimed is:

1. A fluoroscopy apparatus comprising:
 - an illumination portion having a light source that radiates illumination light and excitation light onto a subject;
 - a fluorescence-imaging unit that acquires a fluorescence image by imaging fluorescence generated at the subject by the radiation of the excitation light from the illumination portion;

25

a return-light imaging unit that acquires a reference image by imaging return light returning from the subject by the radiation of the illumination light from the illumination portion; and
 an image-correction unit that corrects the fluorescence image acquired by the fluorescence-imaging unit by using the reference image acquired by the return-light imaging unit,
 wherein in the image-correction unit, a correction fluorescence image is obtained by raising a luminance value of the fluorescence image to the power of the reciprocal of a first exponent that is obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the fluorescence image acquired by the fluorescence-imaging unit when the excitation light of a prescribed intensity is radiated towards the subject; a correction reference image is obtained by raising a luminance value of the reference image to the power of the reciprocal of a second exponent that is obtained by a power approximation of a characteristic of luminance versus distance from the illumination portion to the subject, for the reference image obtained by the return-light imaging unit when the illumination light of a prescribed intensity is radiated towards the subject; and a corrected fluorescence image is obtained by dividing the correction fluorescence image by the correction reference image.

2. A fluoroscopy apparatus according to claim 1, wherein the image-correction unit further raises the luminance value of the corrected fluorescence image to the power of the first exponent.

3. A fluoroscopy apparatus according to claim 1, further comprising an image-acquisition condition adjusting portion that adjusts an image acquisition condition on the basis of the luminance value of the fluorescence image acquired by the fluorescence-imaging unit,
 wherein the image-correction unit normalizes the luminance of the fluorescence image by the image acquisition condition.

4. A fluoroscopy apparatus according to claim 3, wherein the image-acquisition condition adjusting portion adjusts an exposure time of the fluorescence-imaging unit, and the image-correction unit divides the luminance value of the fluorescence image by the exposure time.

5. A fluoroscopy apparatus according to claim 3, wherein the image-acquisition condition adjusting portion adjusts a gain factor of the fluorescence-imaging unit, and the image-correction unit divides the luminance value of the fluorescence image by the gain factor.

6. A fluoroscopy apparatus according to claim 3, wherein the image-acquisition condition adjusting portion adjusts excitation-light intensity from the illumination portion, and the image-correction unit divides the luminance value of the fluorescence image by the excitation-light intensity.

7. A fluoroscopy apparatus according to claim 1, further comprising an image-acquisition condition adjusting portion that adjusts the image acquisition condition on the basis of the luminance value of the reference image acquired by the return-light imaging unit,
 wherein the image-correction unit normalizes the luminance of the reference image by the image acquisition condition.

8. A fluoroscopy apparatus according to claim 7, wherein the image-acquisition condition adjusting portion adjusts an exposure time of the return-light imaging unit, and the image-correction unit divides the luminance value of the reference image by the exposure time.

26

9. A fluoroscopy apparatus according to claim 7, wherein the image-acquisition condition adjusting portion adjusts a gain factor of the return-light imaging unit, and the image-correction unit divides the luminance value of the reference image by the gain factor.

10. A fluoroscopy apparatus according to claim 7, wherein the image-acquisition condition adjusting portion adjusts illumination light intensity from the illumination portion, and the image-correction unit divides the luminance value of the reference image by the illumination light intensity.

11. A fluoroscopy system comprising a fluoroscopy apparatus according to claim 1 and a calibration device that calibrates the fluoroscopy apparatus,
 wherein the calibration device is provided with a standard specimen and an observation-state setting mechanism that changeably sets an observation distance of the fluoroscopy apparatus relative to the standard specimen, and wherein the fluoroscopy apparatus or the calibration device is provided with an exponent calculating unit that calculates the first exponent and the second exponent on the basis of the observation distance set by the observation-state setting mechanism and the fluorescence image and the reference image acquired by imaging the standard specimen with the fluoroscopy apparatus.

12. A fluoroscopy apparatus according to claim 2, further comprising an image-acquisition condition adjusting portion that adjusts an image acquisition condition on the basis of the luminance value of the fluorescence image acquired by the fluorescence-imaging unit,
 wherein the image-correction unit normalizes the luminance of the fluorescence image by the image acquisition condition.

13. A fluoroscopy apparatus according to claim 2, further comprising an image-acquisition condition adjusting portion that adjusts the image acquisition condition on the basis of the luminance value of the reference image acquired by the return-light imaging unit,
 wherein the image-correction unit normalizes the luminance of the reference image by the image acquisition condition.

14. A fluoroscopy system comprising a fluoroscopy apparatus according to claim 2 and a calibration device that calibrates the fluoroscopy apparatus,
 wherein the calibration device is provided with a standard specimen and an observation-state setting mechanism that changeably sets an observation distance of the fluoroscopy apparatus relative to the standard specimen, and wherein the fluoroscopy apparatus or the calibration device is provided with an exponent calculating unit that calculates the first exponent and the second exponent on the basis of the observation distance set by the observation-state setting mechanism and the fluorescence image and the reference image acquired by imaging the standard specimen with the fluoroscopy apparatus.

15. A fluoroscopy apparatus according to claim 12, wherein the image-acquisition condition adjusting portion adjusts an exposure time of the fluorescence-imaging unit, and
 the image-correction unit divides the luminance value of the fluorescence image by the exposure time.

16. A fluoroscopy apparatus according to claim 12, wherein the image-acquisition condition adjusting portion adjusts a gain factor of the fluorescence-imaging unit, and the image-correction unit divides the luminance value of the fluorescence image by the gain factor.

17. A fluoroscopy apparatus according to claim 12, wherein the image-acquisition condition adjusting portion adjusts excitation-light intensity from the illumination portion, and the image-correction unit divides the luminance value of the fluorescence image by the excitation-light intensity. 5

18. A fluoroscopy apparatus according to claim 13, wherein the image-acquisition condition adjusting portion adjusts an exposure time of the return-light imaging unit, and the image-correction unit divides the luminance value of 10 the reference image by the exposure time.

19. A fluoroscopy apparatus according to claim 13, wherein the image-acquisition condition adjusting portion adjusts a gain factor of the return-light imaging unit, and the image-correction unit divides the luminance value of 15 the reference image by the gain factor.

20. A fluoroscopy apparatus according to claim 13, wherein the image-acquisition condition adjusting portion adjusts illumination light intensity from the illumination portion, and 20 the image-correction unit divides the luminance value of the reference image by the illumination light intensity.

* * * * *