



US008747435B2

(12) **United States Patent**  
**Yassinzadeh**

(10) **Patent No.:** **US 8,747,435 B2**  
(45) **Date of Patent:** **Jun. 10, 2014**

(54) **DRUG ELUTING VASCULAR CLOSURE DEVICES AND METHODS**

(75) Inventor: **Zia Yassinzadeh**, San Jose, CA (US)

(73) Assignee: **Cardiva Medical, Inc.**, Sunnyvale, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 130 days.

(21) Appl. No.: **12/711,132**

(22) Filed: **Feb. 23, 2010**

(65) **Prior Publication Data**

US 2010/0145383 A1 Jun. 10, 2010

**Related U.S. Application Data**

(62) Division of application No. 11/302,951, filed on Dec. 13, 2005, now Pat. No. 7,691,127.

(51) **Int. Cl.**  
**A61B 17/08** (2006.01)

(52) **U.S. Cl.**  
USPC ..... **606/213**; 606/214; 606/232

(58) **Field of Classification Search**  
USPC ..... 606/213, 214, 215, 216, 151, 191, 194, 606/232

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,744,364 A	5/1988	Kensey
4,852,568 A	8/1989	Kensey
4,890,612 A	1/1990	Kensey
4,895,168 A	1/1990	Machek
5,061,274 A	10/1991	Kensey
5,108,420 A	4/1992	Marks

5,108,421 A	4/1992	Fowler
5,129,882 A *	7/1992	Weldon et al. .... 604/93.01
5,171,259 A	12/1992	Inoue
5,197,971 A	3/1993	Bonutti
5,222,974 A	6/1993	Kensey et al.
5,258,000 A	11/1993	Gianturco

(Continued)

**FOREIGN PATENT DOCUMENTS**

WO	WO 92/22252	12/1992
WO	WO 95/05121	2/1995

(Continued)

**OTHER PUBLICATIONS**

International search report and written opinion dated Mar. 3, 2008 for PCT/US2006/061119.

(Continued)

*Primary Examiner* — Corrine M McDermott


*Assistant Examiner* — Jing Ou

(74) *Attorney, Agent, or Firm* — Wilson Sonsini Goodrich & Rosati

(57) **ABSTRACT**

Drug eluting vascular closure devices and methods for closing a blood vessel puncture site disposed at a distal end of a tissue tract are described. The devices and methods rely on a combination of the body's own natural mechanism to achieve hemostasis with bio-chemical agents to accelerate the hemostatic process. One method includes the steps of introducing a closure device through the tissue tract and deploying an expansible member at a distal end of the device within the blood vessel to occlude the puncture site. A bio-chemical sealing member disposed proximal the expansible member is then displaced so as to expose a bio-chemical region or release region of the device. At least one bio-chemical agent is thereafter released from the device and into the tissue tract to accelerate the occlusion process in the tract.

**16 Claims, 7 Drawing Sheets**

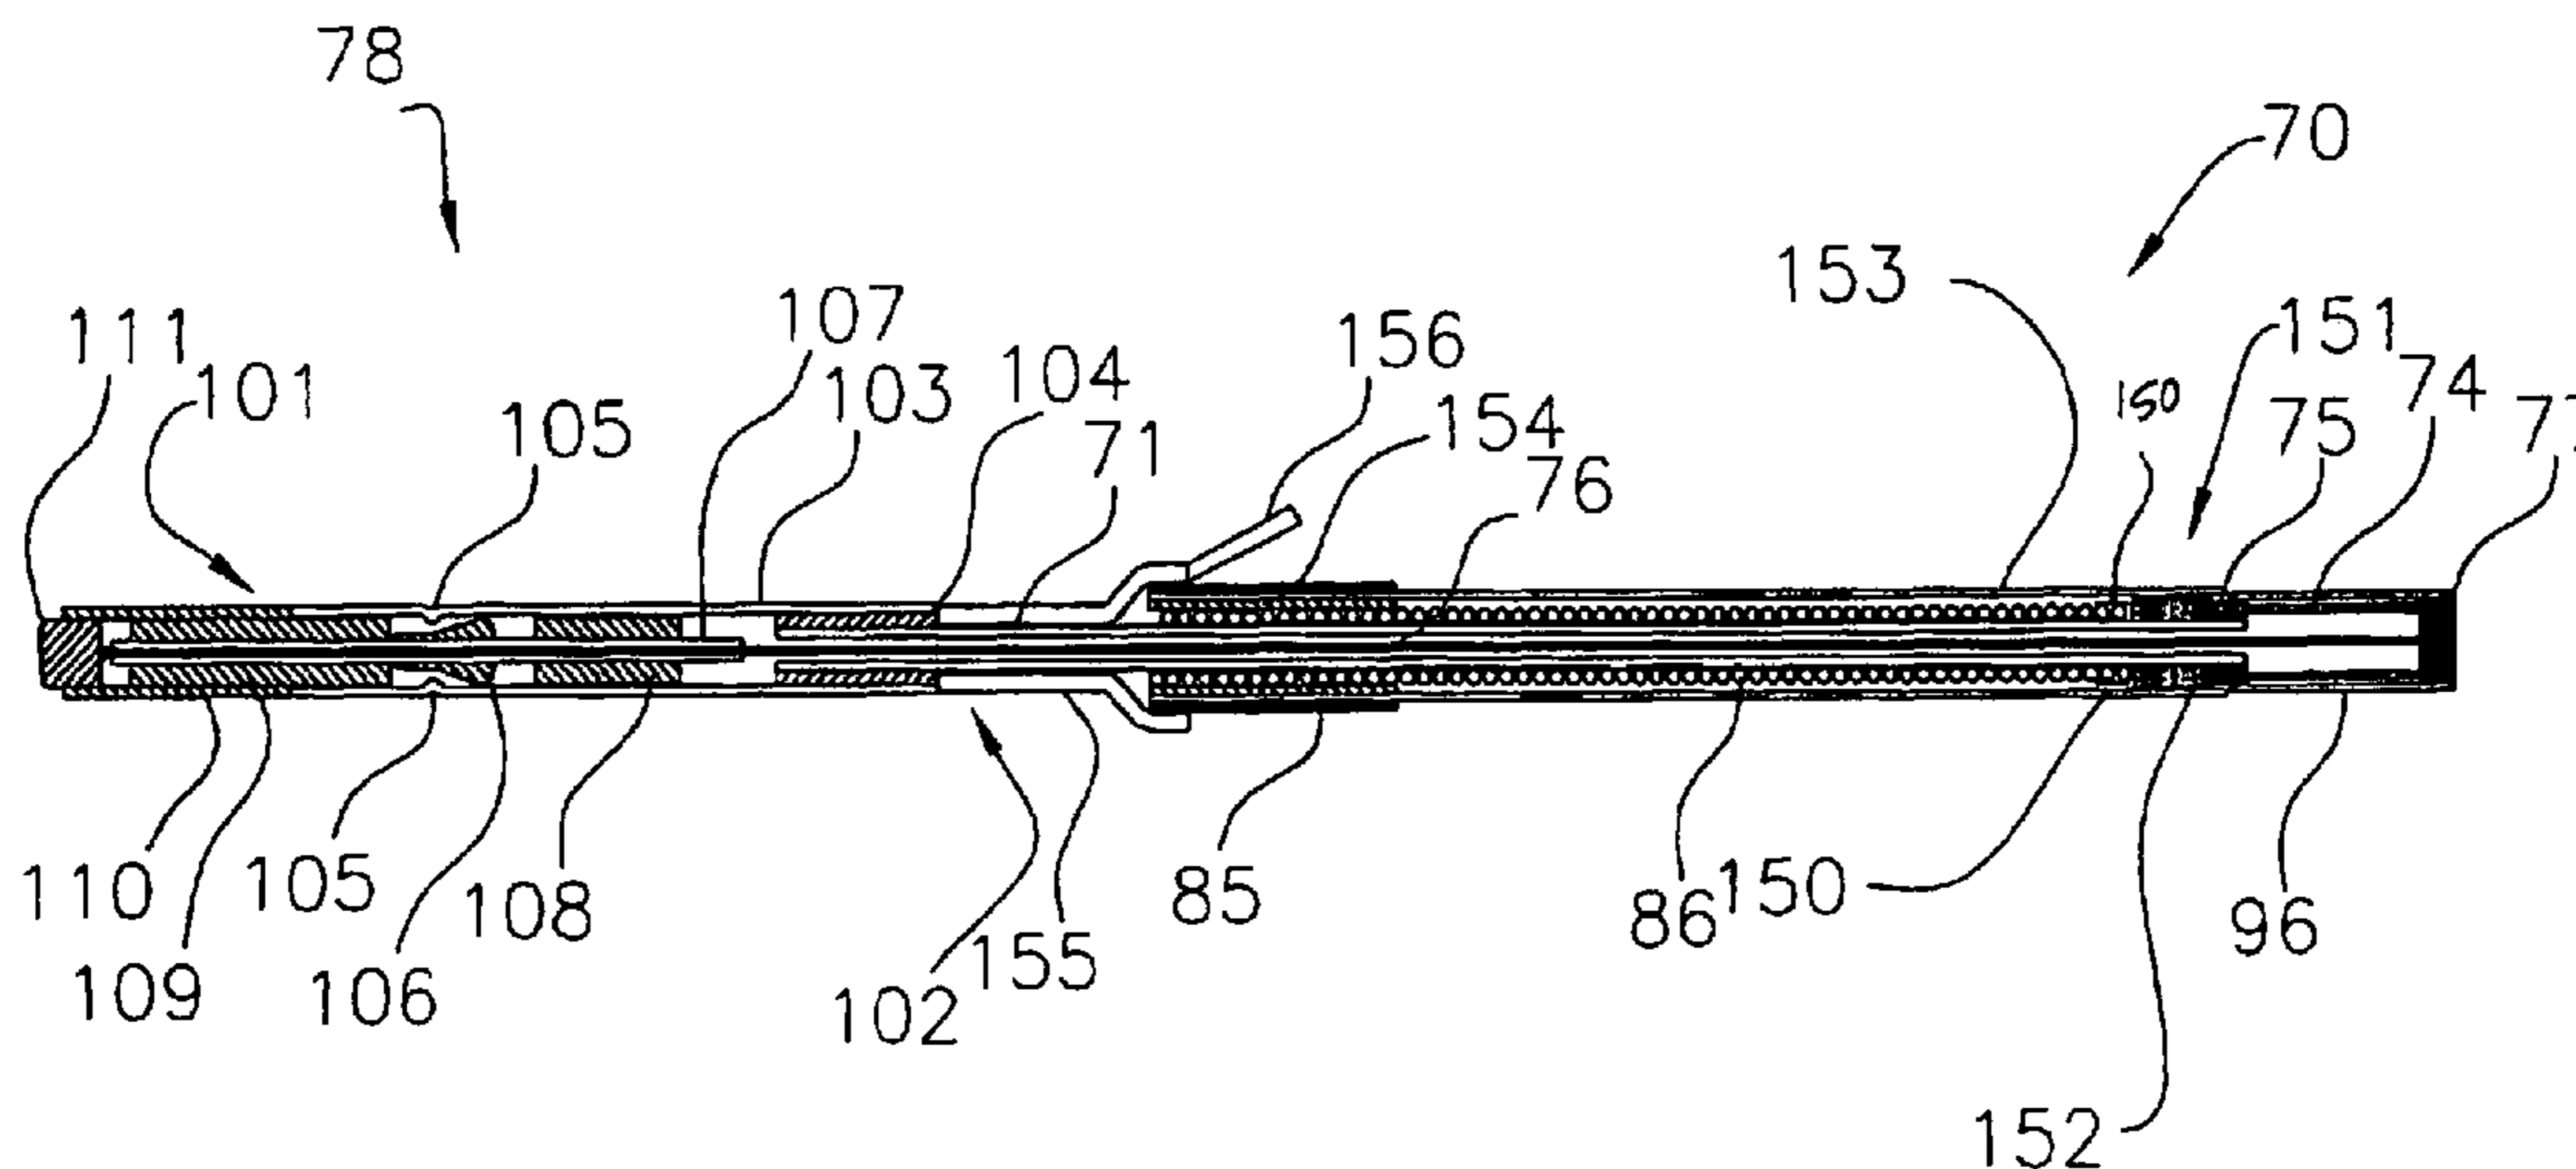

(56)

References Cited

U.S. PATENT DOCUMENTS

5,290,552 A 3/1994 Sierra et al.  
 5,292,332 A 3/1994 Lee  
 5,383,896 A 1/1995 Gershony et al.  
 5,419,765 A 5/1995 Weldon et al.  
 5,454,833 A 10/1995 Boussignac et al.  
 5,456,667 A 10/1995 Ham et al.  
 5,456,689 A 10/1995 Kresch et al.  
 5,486,195 A 1/1996 Myers et al.  
 5,507,744 A 4/1996 Tay et al.  
 5,540,715 A 7/1996 Katsaros et al.  
 5,545,178 A \* 8/1996 Kensey et al. .... 606/213  
 5,549,633 A \* 8/1996 Evans et al. .... 606/139  
 5,626,601 A 5/1997 Gershony et al.  
 5,630,833 A 5/1997 Katsaros et al.  
 5,634,936 A 6/1997 Linden et al.  
 5,649,959 A 7/1997 Hannam et al.  
 5,653,730 A 8/1997 Hammerslag  
 5,725,551 A 3/1998 Myers et al.  
 5,728,133 A 3/1998 Kontos  
 5,728,134 A 3/1998 Barak  
 5,782,860 A 7/1998 Epstein et al.  
 5,810,810 A 9/1998 Tay et al.  
 5,836,913 A 11/1998 Orth et al.  
 5,851,210 A 12/1998 Torossian  
 5,861,003 A 1/1999 Latson et al.  
 5,868,778 A 2/1999 Gershony et al.  
 5,895,398 A 4/1999 Wensel et al.  
 5,922,009 A 7/1999 Epstein et al.  
 5,935,147 A \* 8/1999 Kensey et al. .... 606/213  
 5,951,583 A 9/1999 Jensen et al.  
 5,951,589 A 9/1999 Epstein et al.  
 5,957,952 A 9/1999 Gershony et al.  
 5,979,453 A 11/1999 Savage et al.  
 6,007,563 A 12/1999 Nash et al.  
 6,012,457 A 1/2000 Lesh  
 6,017,359 A 1/2000 Gershony et al.  
 6,022,361 A 2/2000 Epstein et al.  
 6,045,569 A 4/2000 Kensey et al.  
 6,045,570 A 4/2000 Epstein et al.  
 6,048,358 A 4/2000 Barak  
 6,056,768 A 5/2000 Cates et al.  
 6,056,769 A 5/2000 Epstein et al.  
 6,056,770 A 5/2000 Epstein et al.  
 6,080,182 A 6/2000 Shaw et al.  
 6,126,675 A 10/2000 Shchervinsky et al.  
 6,146,396 A 11/2000 Konya et al.  
 6,162,240 A 12/2000 Cates et al.  
 6,193,670 B1 2/2001 Van Tassel et al.  
 6,248,124 B1 6/2001 Pedros et al.  
 6,296,657 B1 10/2001 Brucker  
 6,464,712 B1 10/2002 Epstein et al.  
 6,569,185 B2 5/2003 Unga  
 6,610,026 B2 8/2003 Cragg et al.  
 6,656,207 B2 12/2003 Epstein et al.  
 6,699,261 B1 3/2004 Cates et al.  
 6,743,195 B2 6/2004 Zucker  
 6,764,467 B1 \* 7/2004 Roby et al. .... 604/191  
 6,818,008 B1 \* 11/2004 Cates et al. .... 606/213  
 6,913,614 B2 7/2005 Marino et al.  
 6,994,686 B2 \* 2/2006 Cruise et al. .... 604/82  
 7,008,441 B2 3/2006 Zucker

7,025,776 B1 4/2006 Houser et al.  
 7,115,127 B2 10/2006 Lindenbaum et al.  
 7,223,266 B2 5/2007 Lindenbaum et al.  
 7,618,438 B2 \* 11/2009 White et al. .... 606/232  
 7,691,127 B2 4/2010 Yassinzadeh  
 2002/0026215 A1 \* 2/2002 Redmond et al. .... 606/213  
 2002/0072767 A1 6/2002 Zhu  
 2002/0133123 A1 9/2002 Zucker  
 2002/0133193 A1 \* 9/2002 Ginn et al. .... 606/216  
 2003/0018357 A1 1/2003 Luthra et al.  
 2003/0045835 A1 3/2003 Anderson et al.  
 2003/0051735 A1 \* 3/2003 Pavcnik et al. .... 128/831  
 2003/0055454 A1 3/2003 Zucker  
 2003/0093116 A1 \* 5/2003 Nowakowski .... 606/215  
 2003/0100921 A1 5/2003 Addis et al.  
 2003/0163146 A1 8/2003 Epstein et al.  
 2003/0191493 A1 10/2003 Epstein et al.  
 2004/0172060 A1 9/2004 Cates et al.  
 2004/0176758 A1 9/2004 Yassinzadeh  
 2004/0176798 A1 9/2004 Epstein et al.  
 2004/0243052 A1 12/2004 Kauphusman et al.  
 2004/0249342 A1 \* 12/2004 Khosravi et al. .... 604/96.01  
 2005/0065549 A1 3/2005 Cates et al.  
 2005/0090860 A1 \* 4/2005 Paprocki .... 606/213  
 2005/0107781 A1 5/2005 Ostrovsky et al.  
 2005/0216054 A1 9/2005 Widomski et al.  
 2005/0228443 A1 10/2005 Yassinzadeh  
 2005/0228444 A1 10/2005 Wendlandt  
 2005/0267522 A1 12/2005 Yassinzadeh et al.  
 2005/0277980 A1 12/2005 Yassinzadeh  
 2006/0034935 A1 2/2006 Pronovost et al.  
 2006/0189972 A1 8/2006 Grossman  
 2006/0229670 A1 10/2006 Bates  
 2007/0032823 A1 \* 2/2007 Tegg .... 606/232  
 2007/0038244 A1 2/2007 Morris et al.  
 2007/0249939 A1 10/2007 Gerbi et al.  
 2007/0276435 A1 11/2007 Yassinzadeh et al.

FOREIGN PATENT DOCUMENTS

WO WO 96/24290 8/1996  
 WO WO 98/34546 8/1998  
 WO WO 98/40017 9/1998  
 WO WO 98/40017 A3 10/1998  
 WO WO 00/06029 2/2000  
 WO WO 00/06031 2/2000

OTHER PUBLICATIONS

International search report and written opinion dated Oct. 2, 2008 for PCT/US2008/068933.  
 Office action dated Feb. 13, 2009 for U.S. Appl. No. 11/302,951.  
 Office action dated Apr. 15, 2011 for U.S. Appl. No. 11/772,718.  
 Office action dated Jun. 22, 2009 for U.S. Appl. No. 11/772,718.  
 Office action dated Jul. 16, 2008 for U.S. Appl. No. 11/302,951.  
 Office action dated Aug. 3, 2009 for U.S. Appl. No. 11/302,951.  
 Office action dated Oct. 26, 2010 for U.S. Appl. No. 11/772,718.  
 Office action dated Nov. 12, 2009 for U.S. Appl. No. 11/772,718.  
 European search report and search opinion dated Apr. 3, 2013 for EP Application No. 06850411.  
 European search report and search opinion dated Jul. 5, 2013 for EP Application No. 08772314.4.

\* cited by examiner



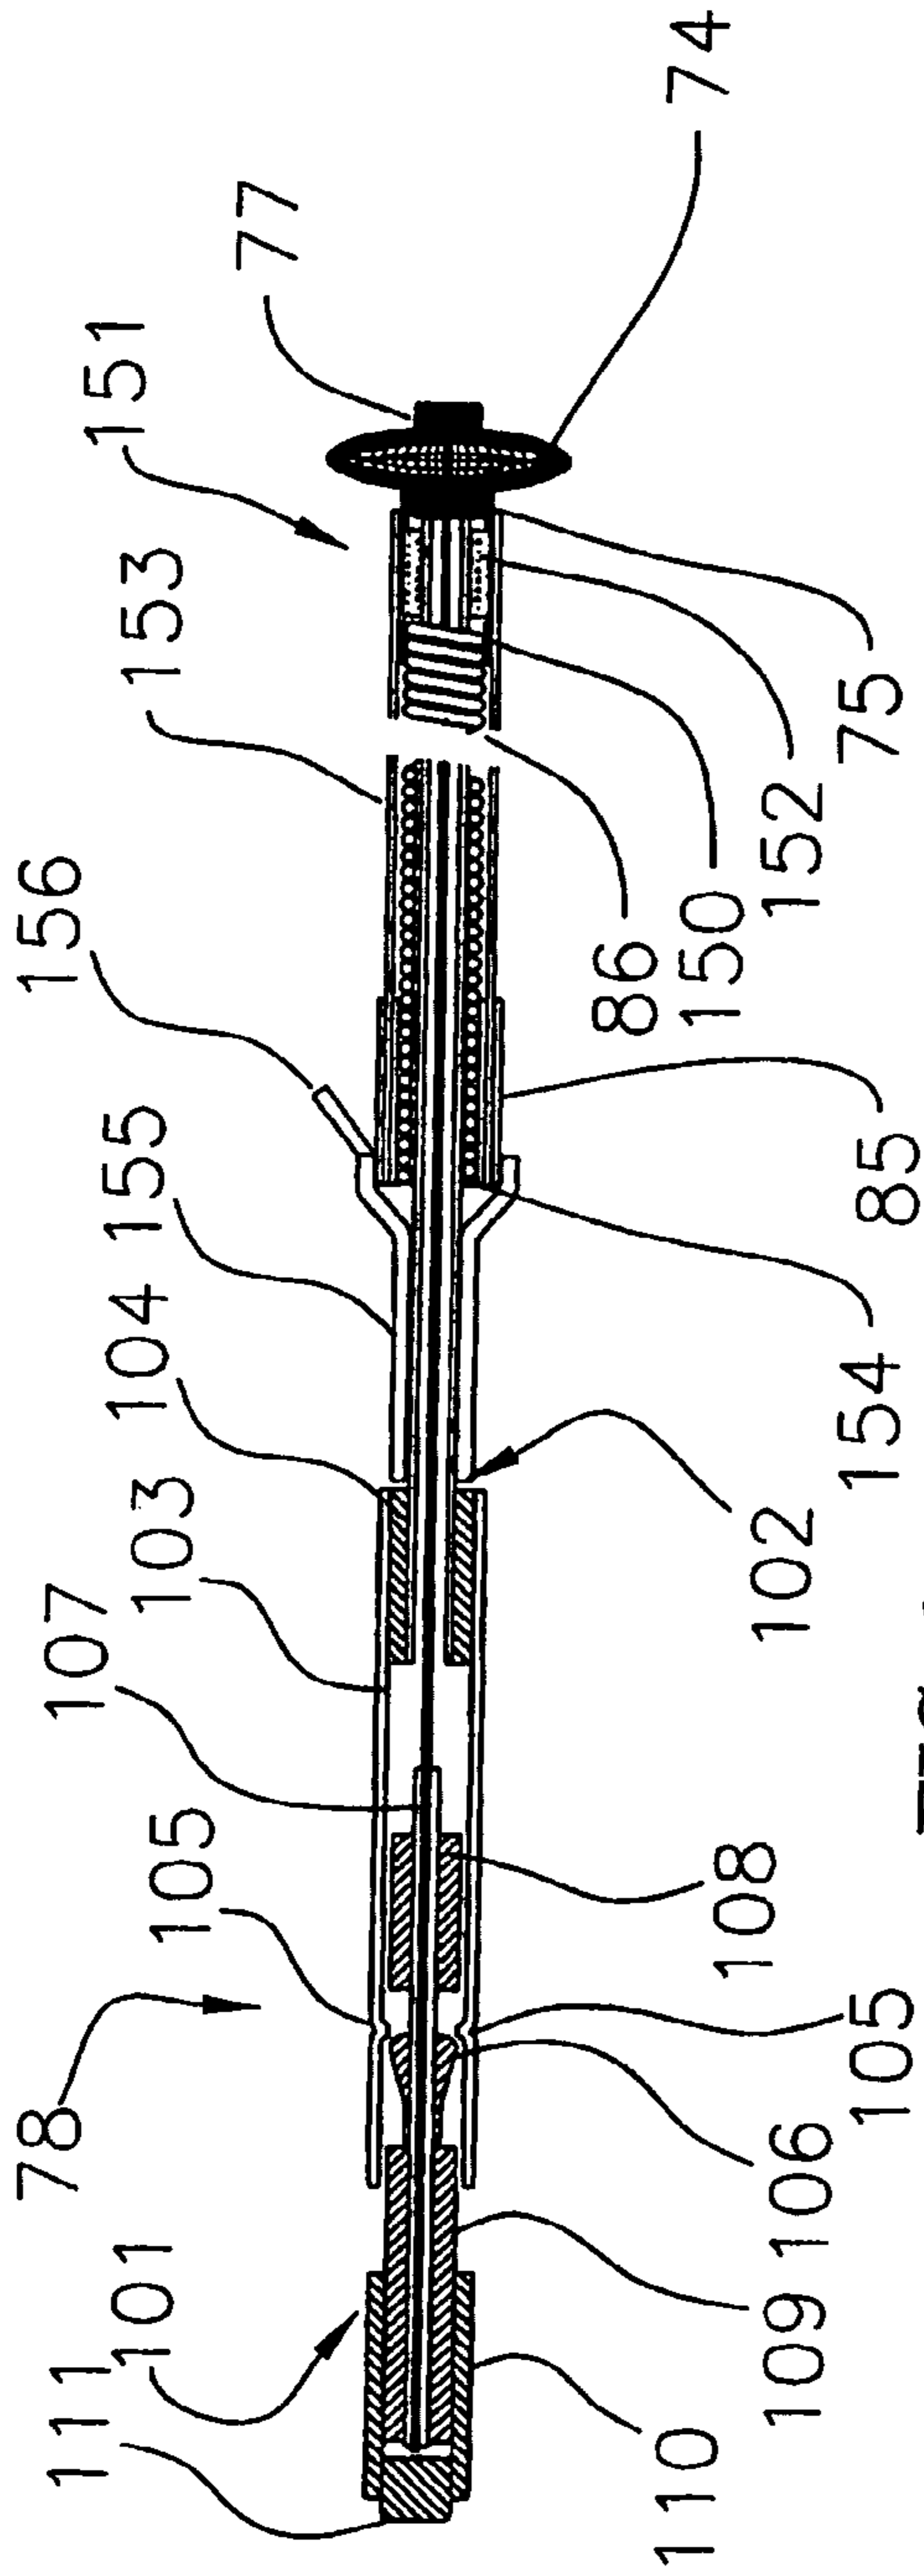


FIG. 3

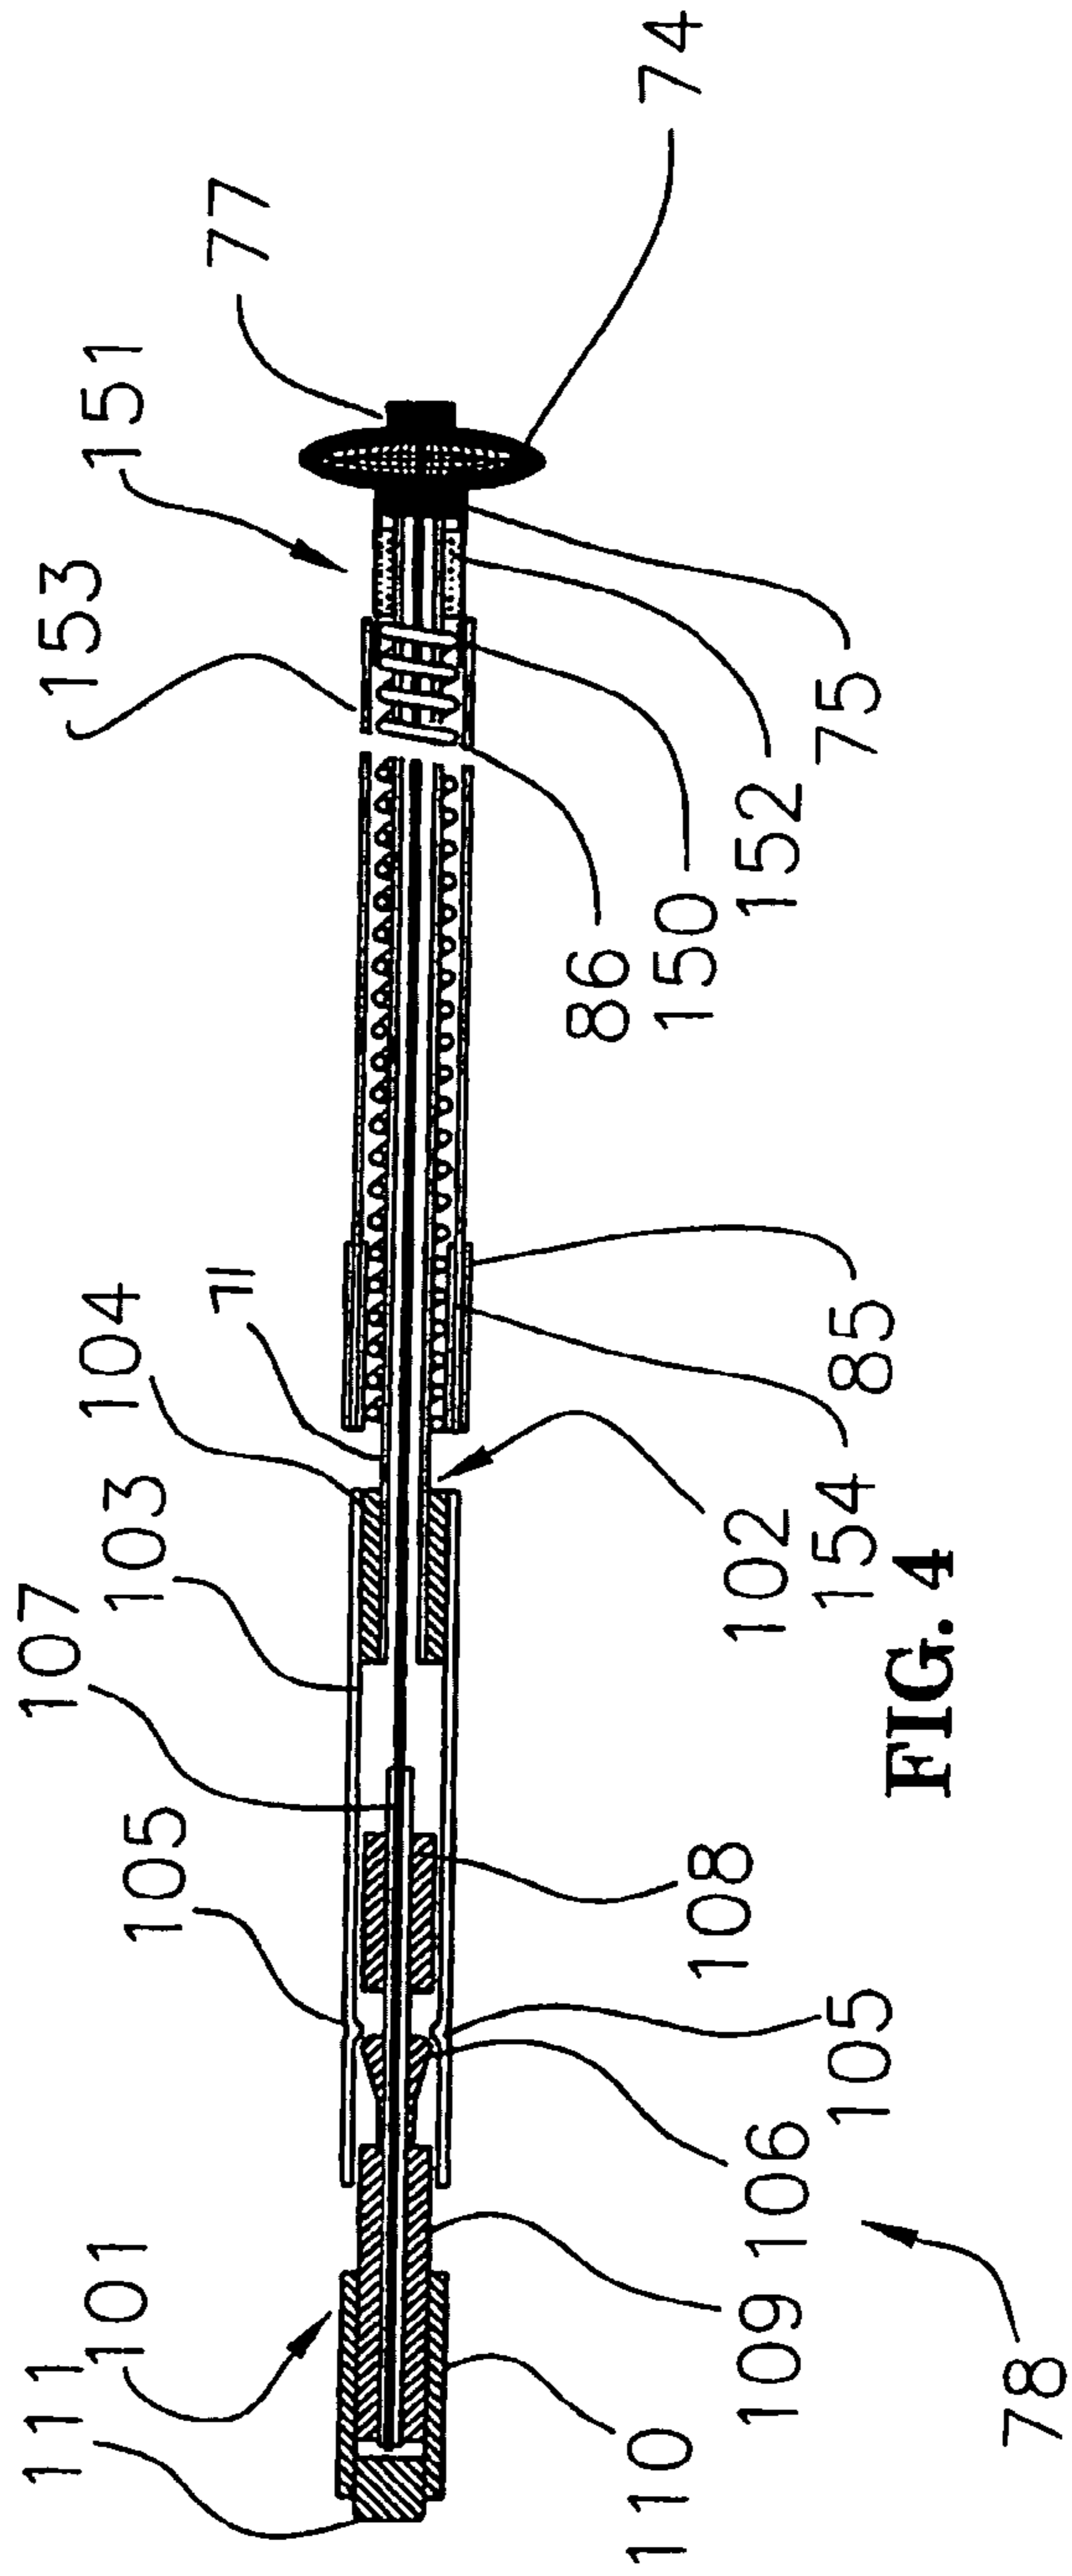


FIG. 4

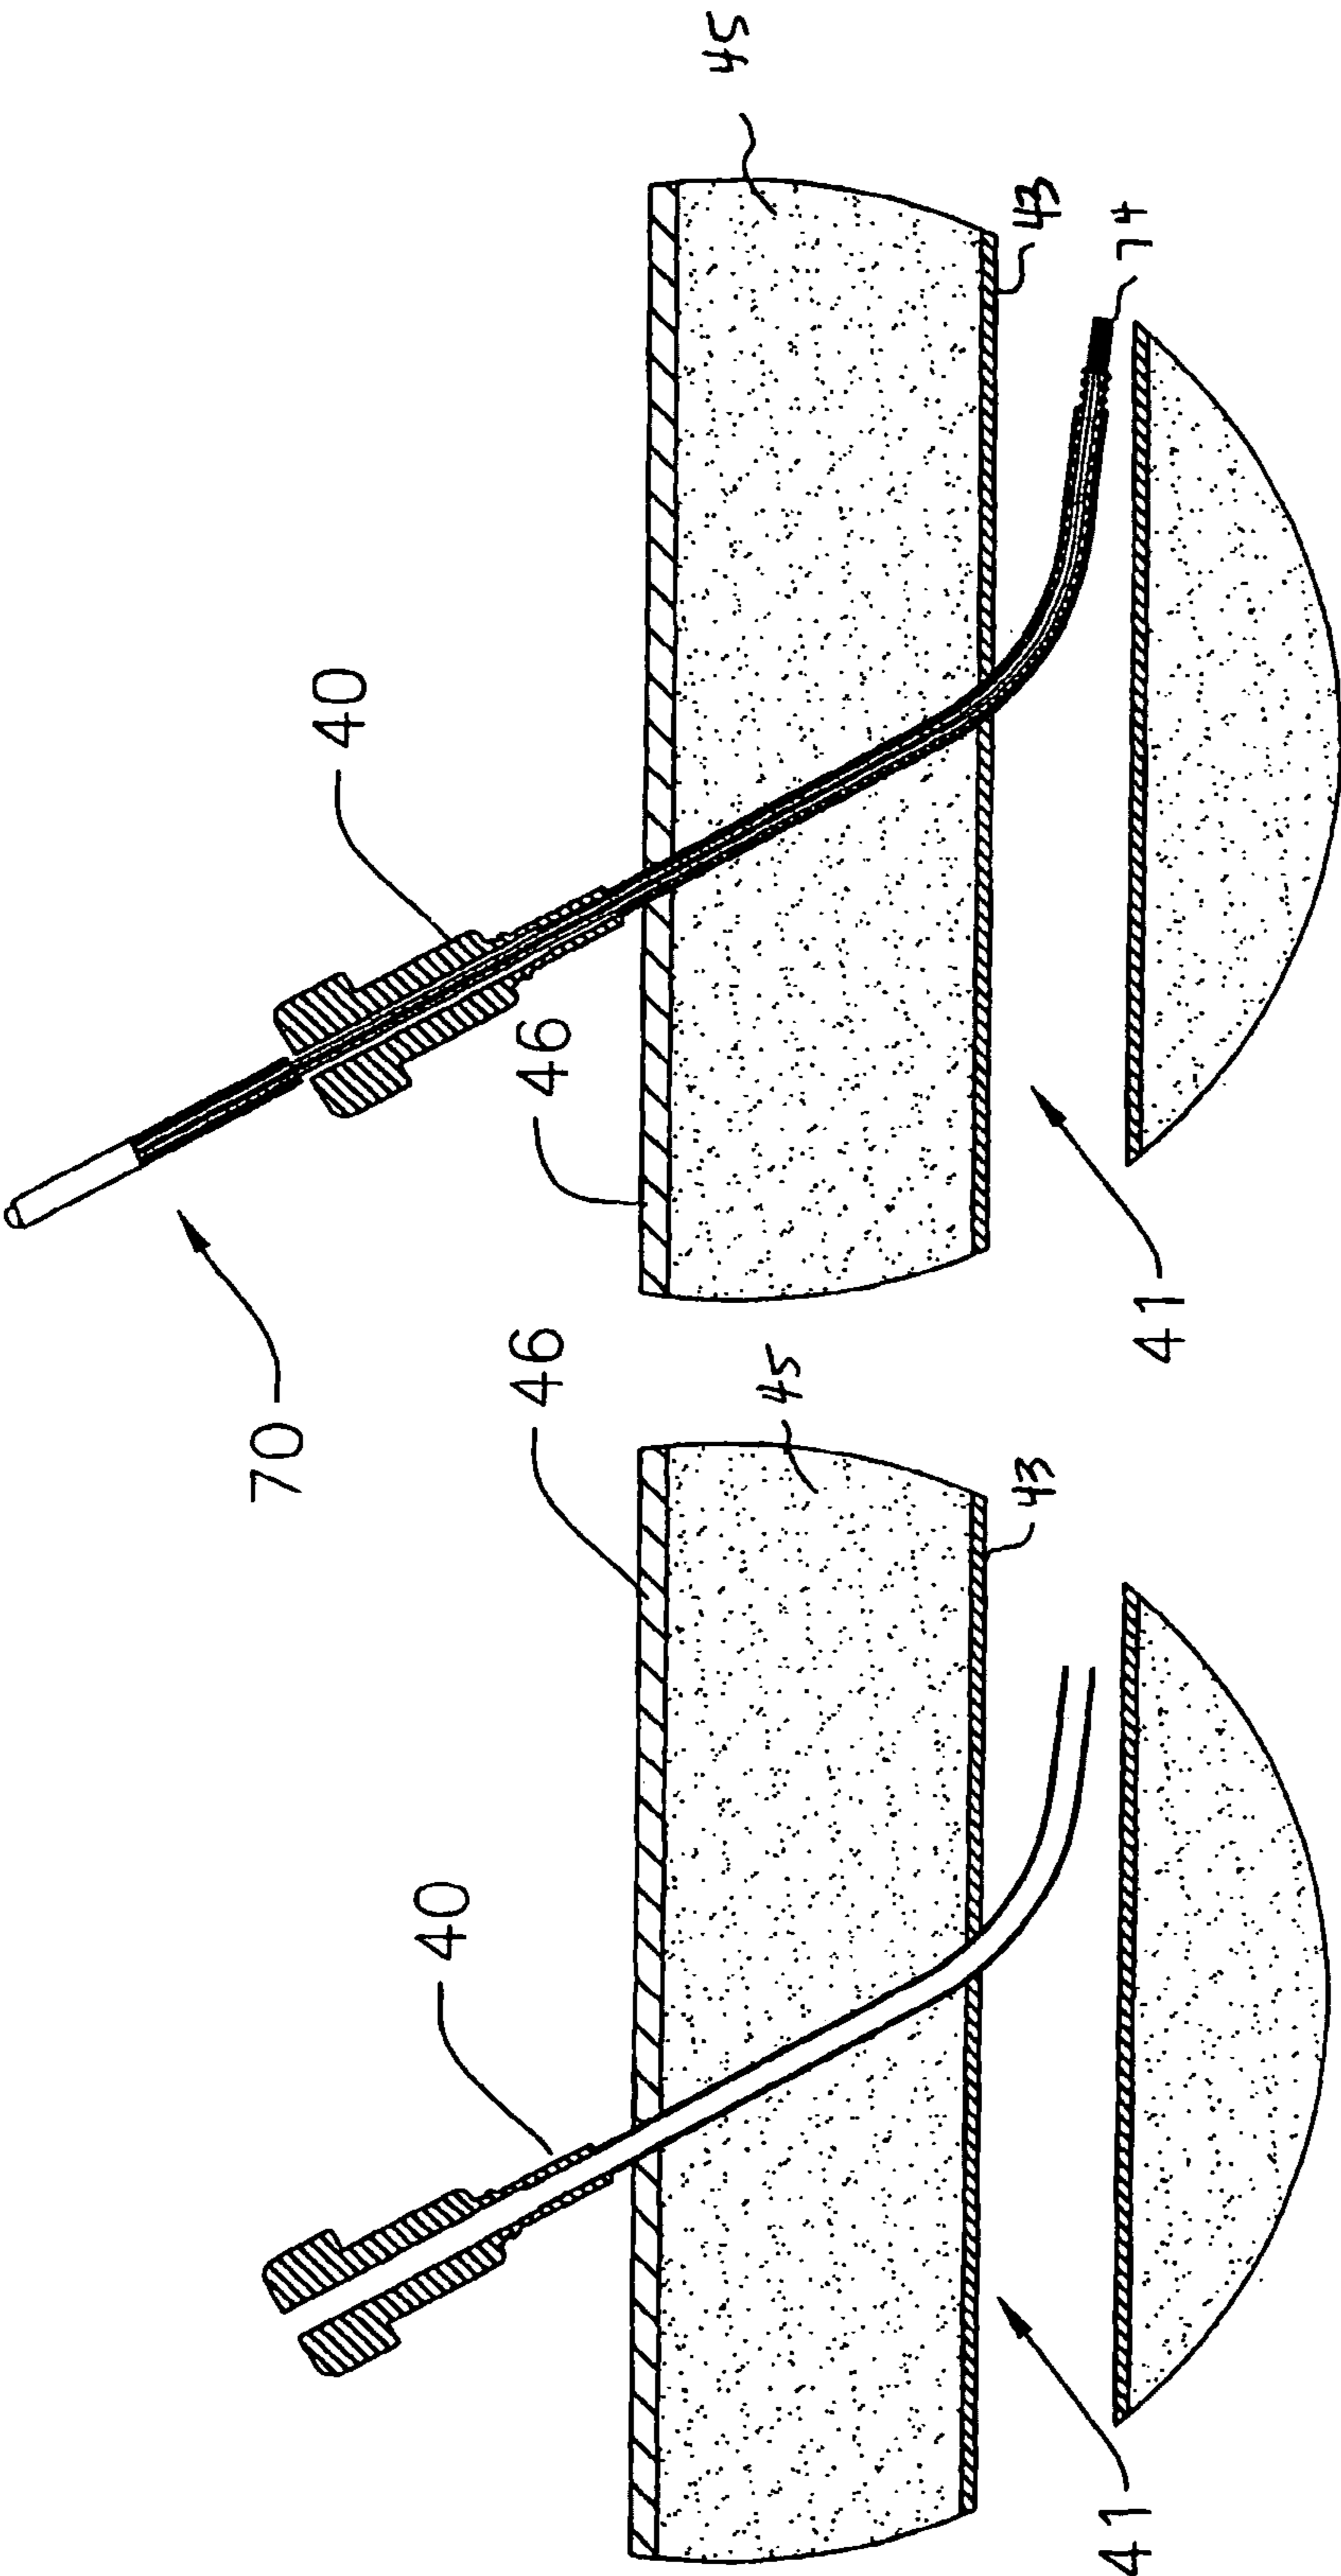


FIG. 5B

FIG. 5A

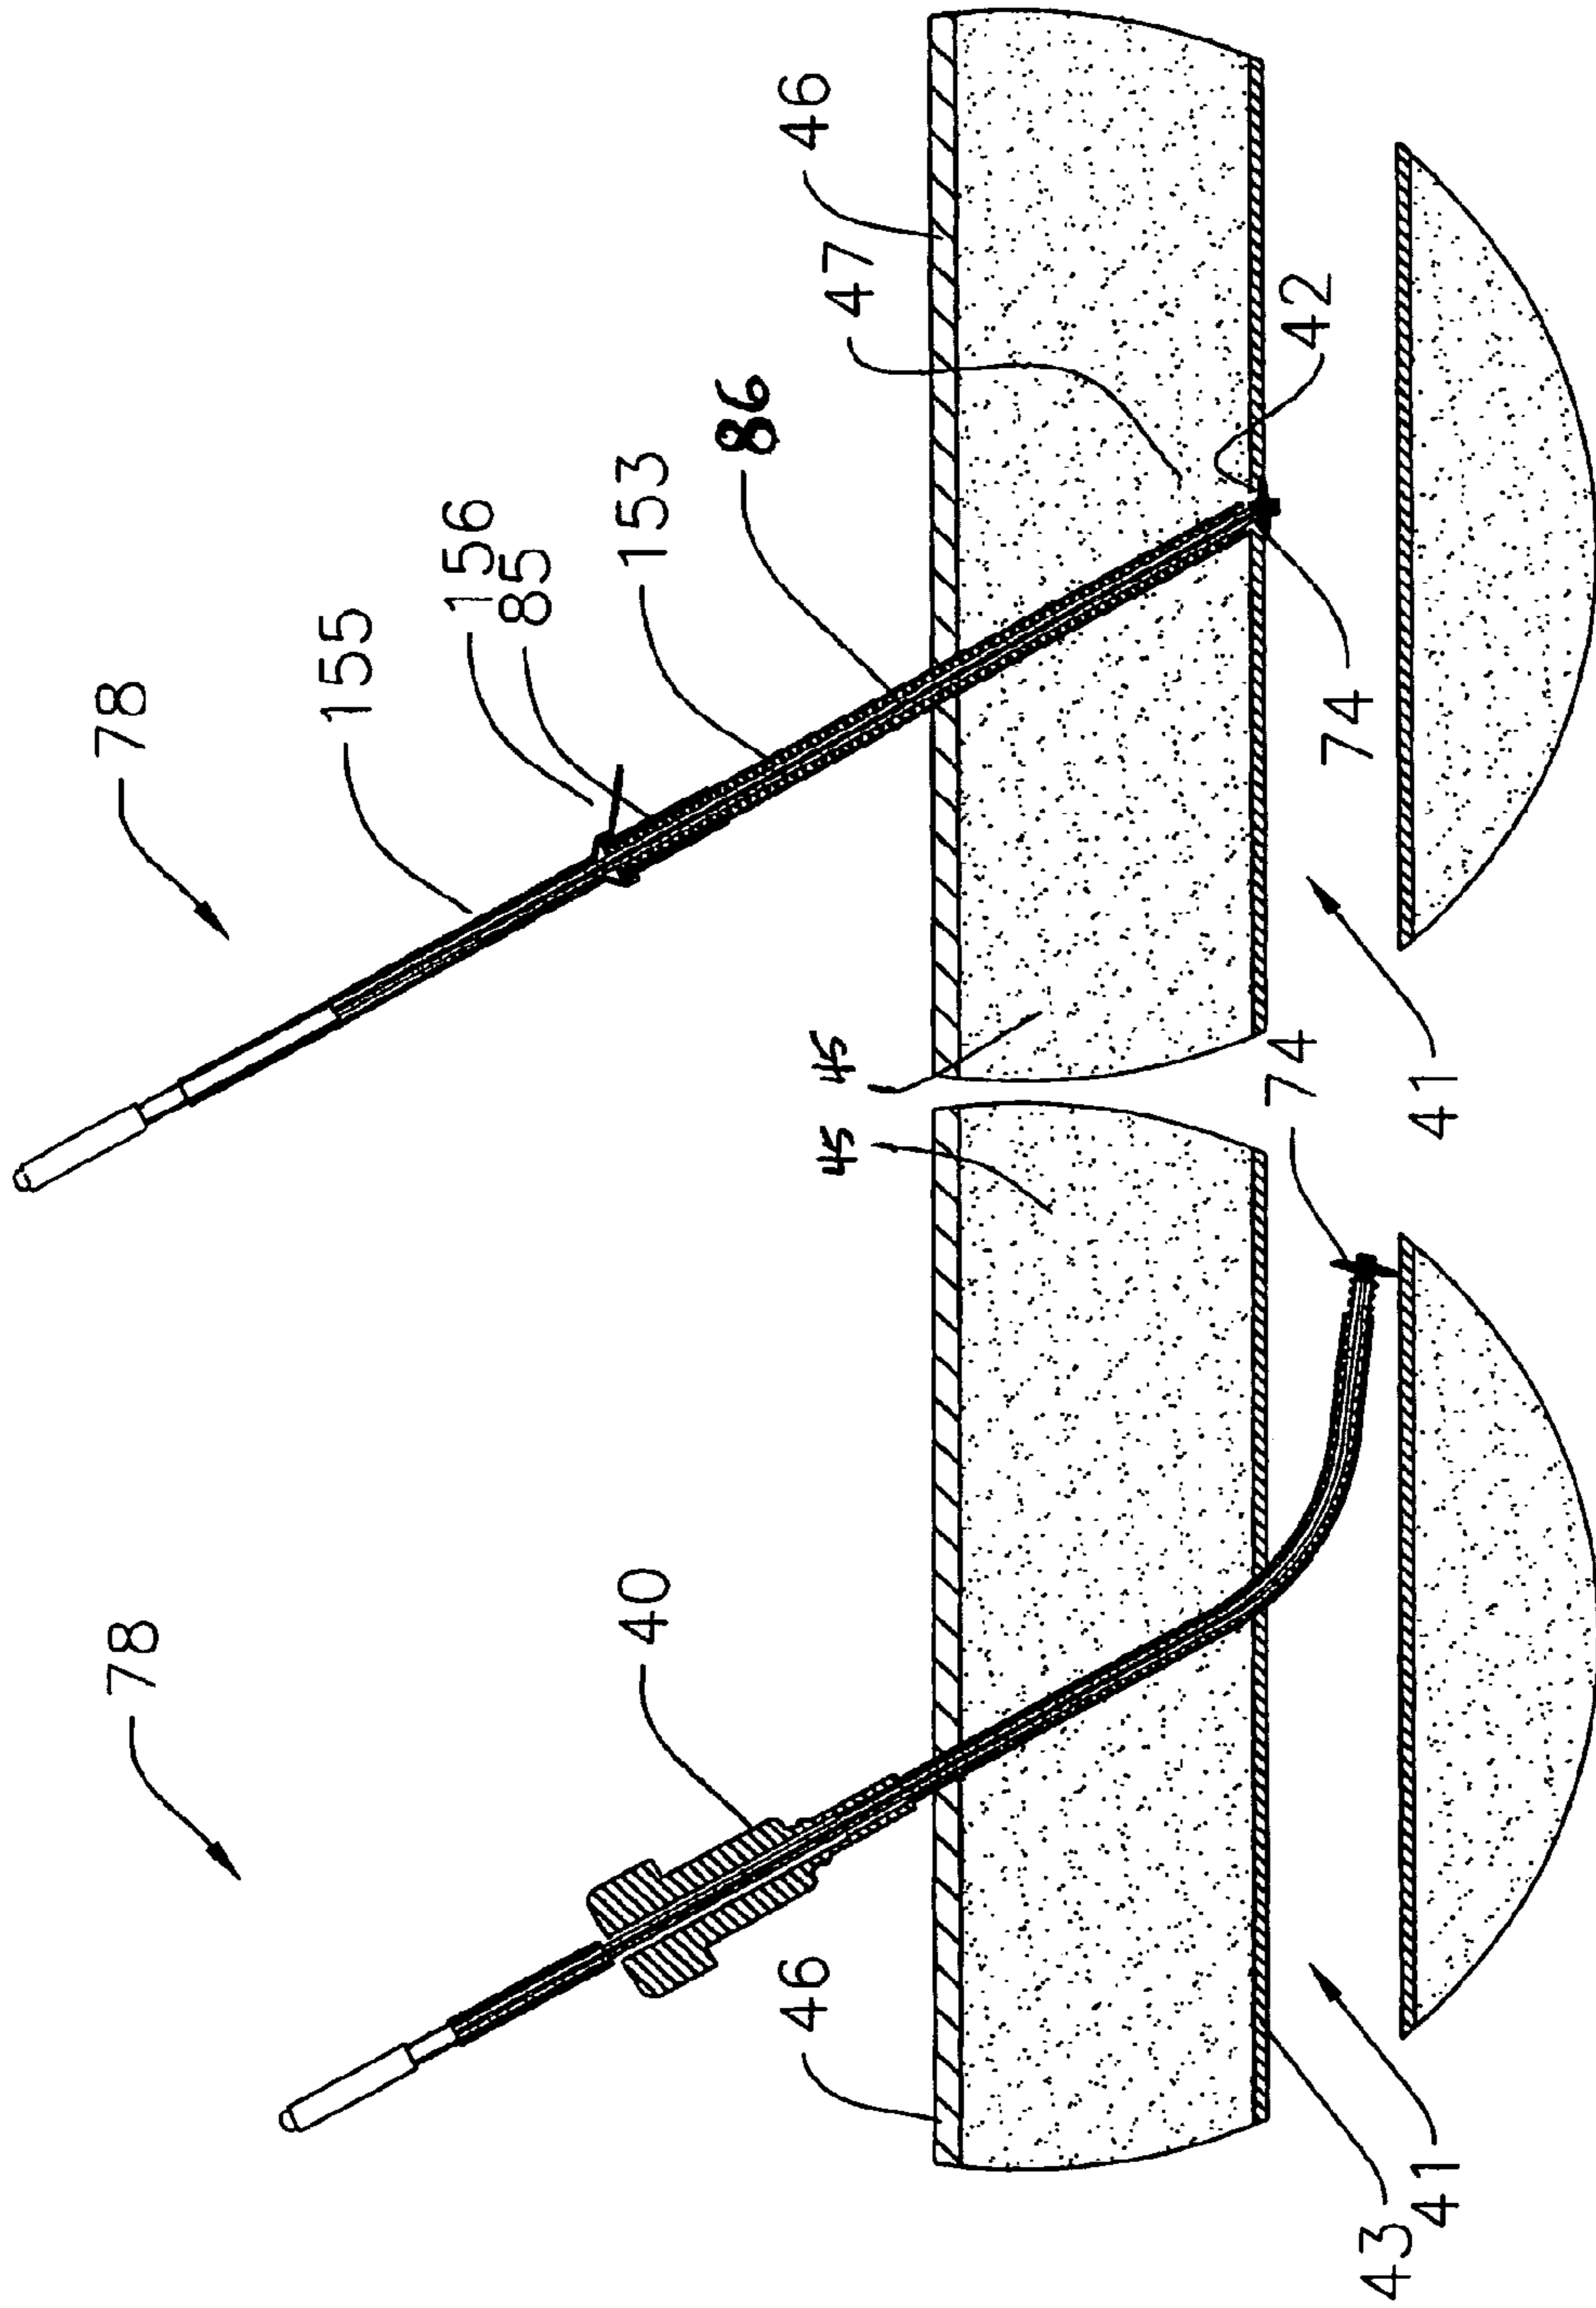


FIG. 5D

FIG. 5C

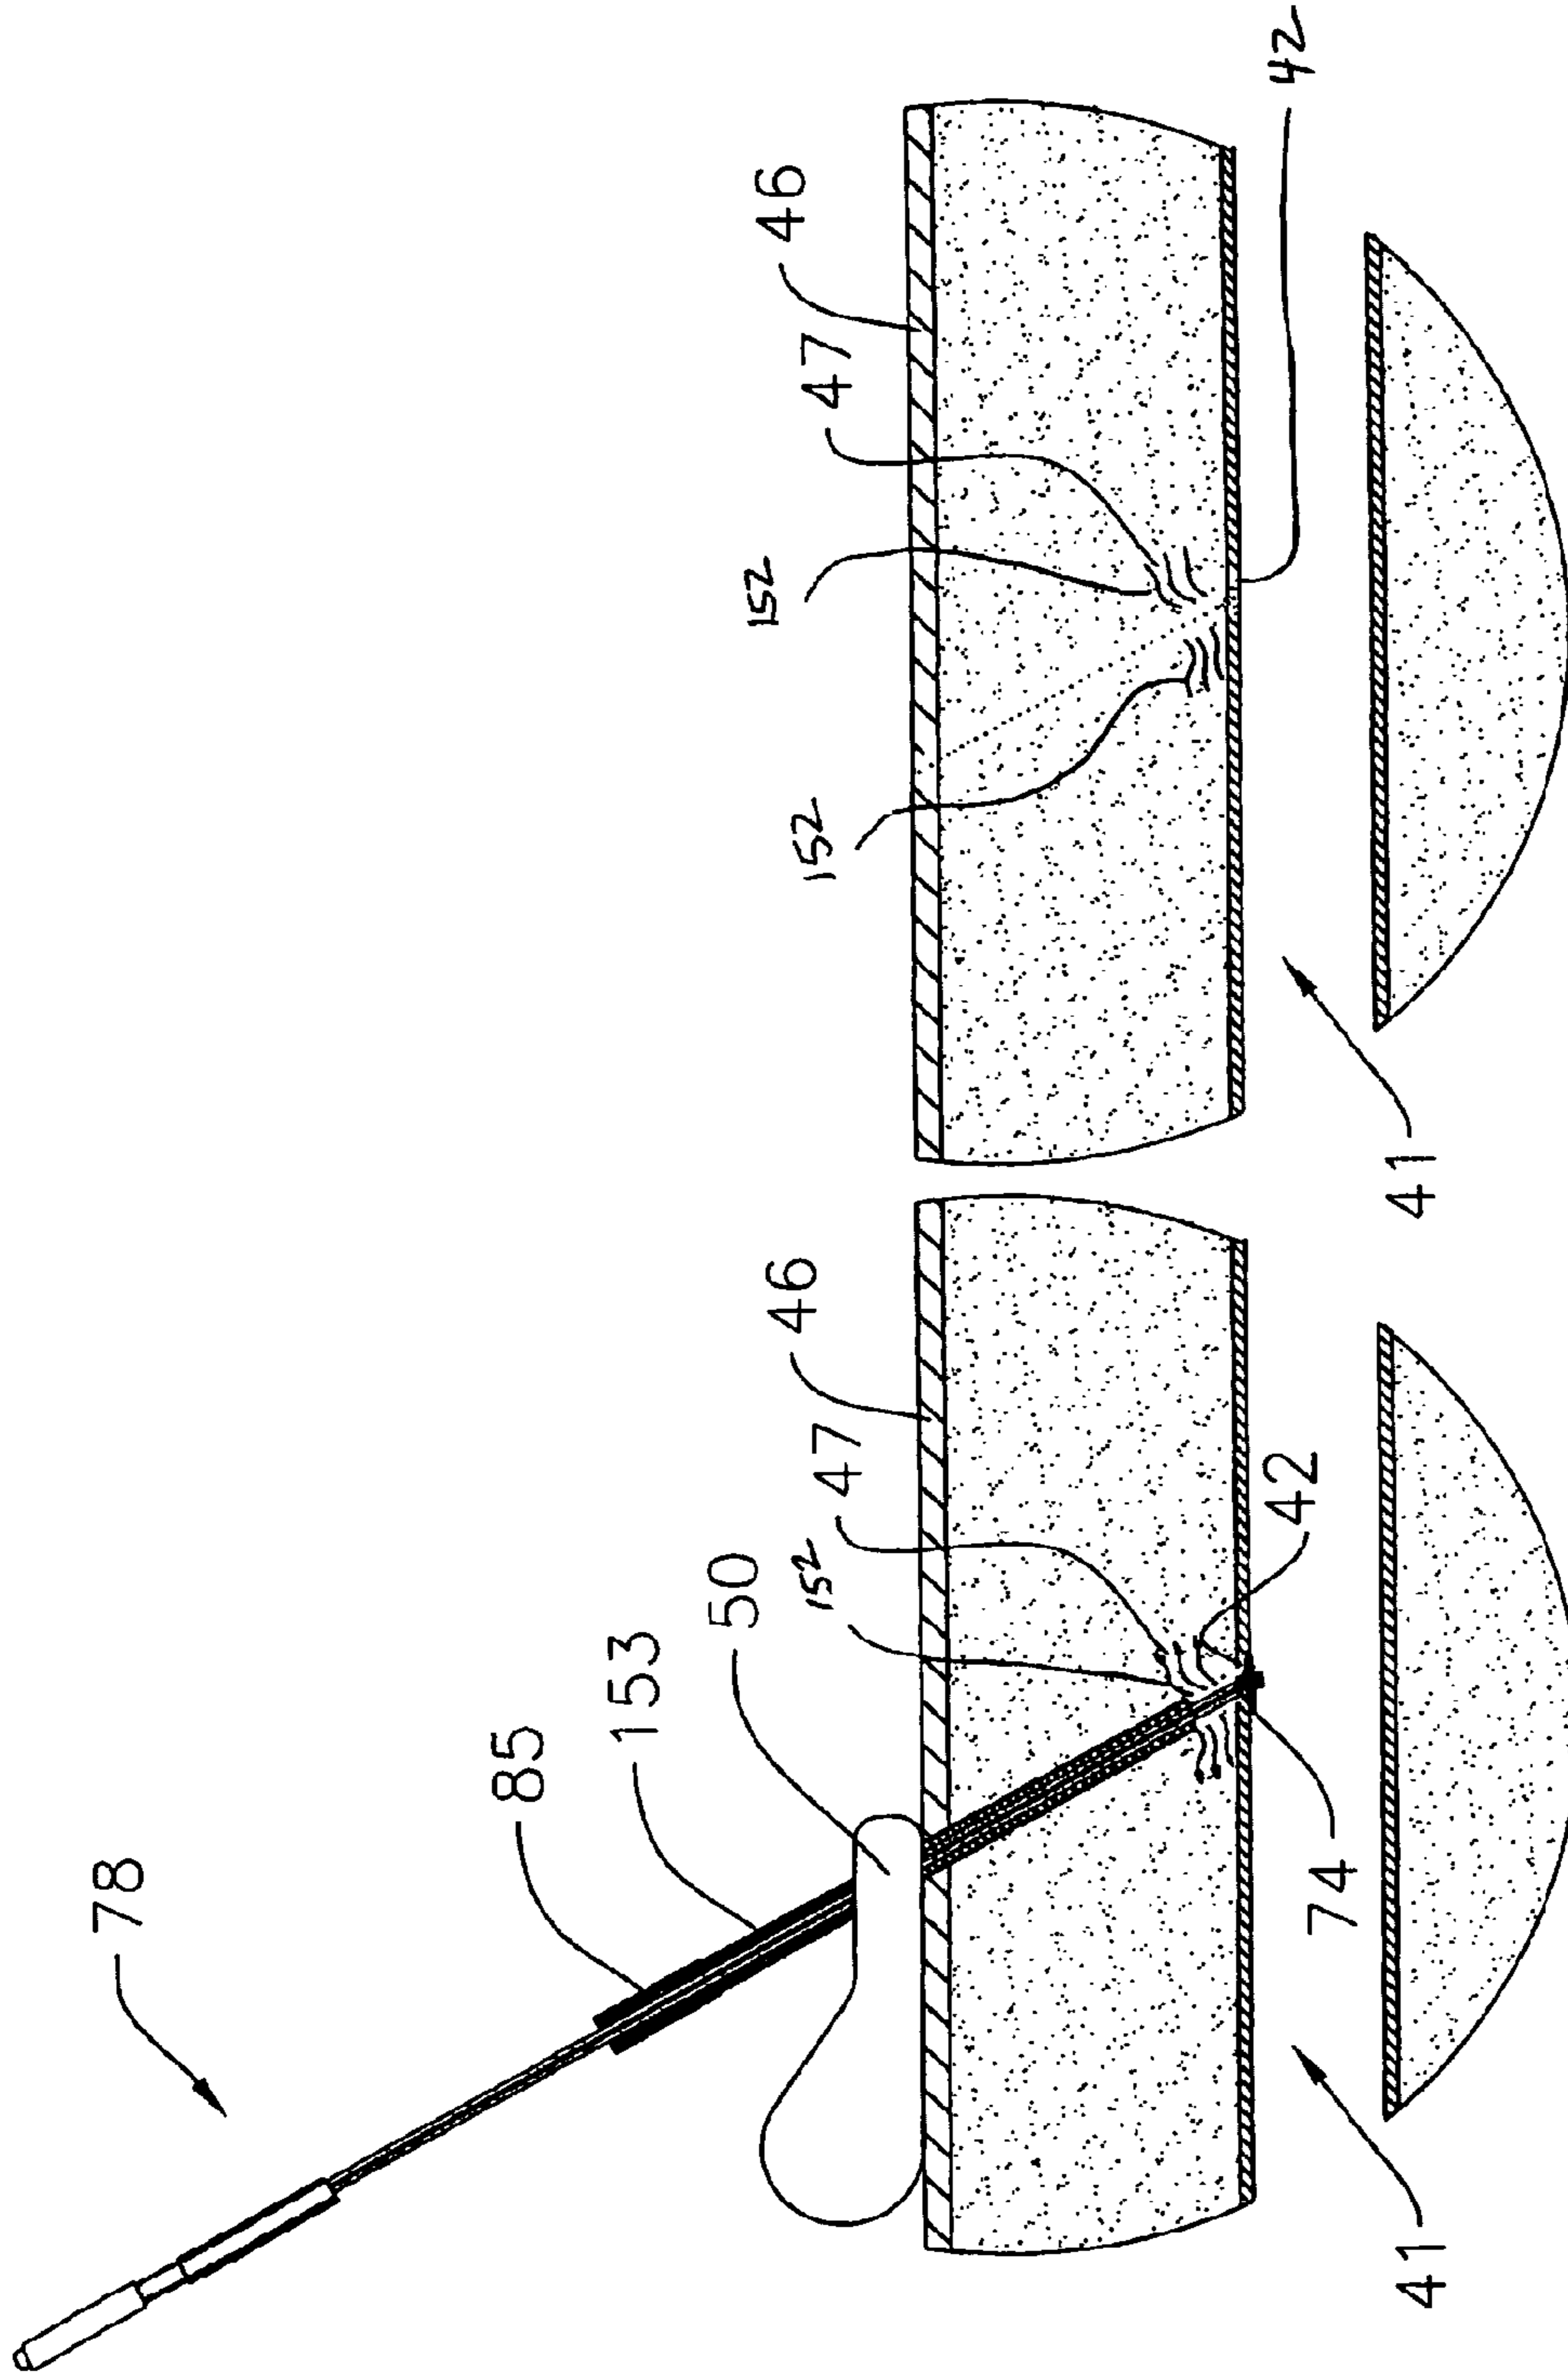


FIG. 5F

FIG. 5E







## DRUG ELUTING VASCULAR CLOSURE DEVICES AND METHODS

### CROSS-REFERENCES TO RELATED APPLICATIONS

This application is a divisional of U.S. patent application Ser. No. 11/302,951 filed Dec. 13, 2005, now U.S. Pat. No. 7,691,127 the full disclosure of which is incorporated herein by reference.

### BACKGROUND OF THE INVENTION

#### 1. Field of the Invention

The present invention relates generally to devices and methods for percutaneous sealing of puncture sites in body lumens or tissue tracts. More specifically, the present invention relates to drug eluting vascular closure devices and methods for hemostasis of vascular puncture sites.

Percutaneous access of blood vessels in the human body is routinely performed for diagnostics or interventional procedures such as coronary and peripheral angiography, angioplasty, atherectomies, placement of vascular stents, coronary retroperfusion and retroinfusion, cerebral angiograms, treatment of strokes, cerebral aneurysms, and the like. Patients undergoing these procedures are often treated with anti-coagulants such as heparin, thrombolytics, and the like, which make the closure and hemostasis process of the puncture site in the vessel wall at the completion of such interventional procedures more difficult to achieve.

Various devices have been introduced to provide hemostasis, however none have been entirely successful. Some devices utilize collagen or other biological plugs to seal the puncture site. Alternatively, sutures and/or staples have also been applied to close the puncture site. External foreign objects such as plugs, sutures, or staples however may cause tissue reaction, inflammation, and/or infection as they all "leave something behind" to achieve hemostasis.

There is also another class of devices that use the body's own natural mechanism to achieve hemostasis wherein no foreign objects are left behind. Such devices typically provide hemostasis by sealing the puncture site from the inside of the vessel wall wherein the device is left in place in the vessel lumen until hemostasis is reached and thereafter removed. Although such safe and simple devices have achieved relative levels of success, they often are slow in achieving complete hemostasis, particularly in highly anti-coagulated patients. As such, such devices are often used as an adjunct to manual compression which still remains to be the most used method in closing the puncture site after the interventional procedure.

There is yet another class of devices where highly thrombogenic substances are mixed and injected to the puncture site for the purpose of accelerating the hemostatic process. These mixtures contain one or more clot promoting substances, such as thrombin and/or fibrinogen, along with other substances, such as collagen. These devices generally work by first occluding the puncture site from the inside of the vessel, usually by use of a balloon, and then injecting the mixture into the tissue tract. The balloon is then removed. Such devices suffer from several drawbacks which may cause severe complications. For example, the occluding member may not be adequate to prevent these highly thrombogenic substances from entering the blood vessel. Further, the injection of the mixture is often not well controlled and highly technique dependant, which again may allow these substances to enter the blood stream.

In light of the above, it would be desirable to provide alternative devices and methods for providing complete hemostasis of a puncture site in a body lumen, particularly blood vessels of the human body. It would be particularly desirable if such devices and methods utilize the body's own natural healing mechanism to achieve hemostasis. It would be further desirable if the natural hemostatic process can be safely accelerated by the controlled use of bio-chemical agents. It would be further desirable if such devices and systems utilize a simple construction and user interface allowing for convenient application without numerous intermediary steps. Further, such devices should be safe and reliable without the need for much user intervention. At least some of these objective will be met by the devices and methods of the present invention described hereinafter.

#### 2. Description of the Background Art

Hemostasis devices for use in blood vessels and tracts in the body are described in pending U.S. patent application Ser. Nos. 10/974,008; 10/857,177; 10/821,633; 10/795,019; and 10/718,504 and U.S. Pat. Nos. 6,656,207; 6,464,712; 6,056,770; 6,056,769; 6,045,570; 6,022,361; 5,951,589; 5,922,009; and 5,782,860, assigned to the assignee of the present application. The following U.S. Patents and Publications may be relevant to the present invention: U.S. Pat. Nos. 4,744,364; 4,852,568; 4,890,612; 5,108,421; 5,171,259; 5,258,000; 5,383,896; 5,419,765; 5,454,833; 5,626,601; 5,630,833; 5,634,936; 5,728,134; 5,836,913; 5,861,003; 5,868,778; 5,951,583; 5,957,952; 6,017,359; 6,048,358; and 6,296,657; U.S. Publication Nos. 2002/0133123; 2003/0055454; 2003/0045835; and 2004/0243052.

The full disclosures of each of the above mentioned references are incorporated herein by reference.

### BRIEF SUMMARY OF THE INVENTION

The present invention provides drug eluting, self-tensioning closure devices and methods for percutaneous access and closure of puncture sites in a body lumen, particularly blood vessels of the human body. It will be appreciated however that application of the present invention is not limited to the blood vasculature, and as such may be applied to any of the vessels, even severely tortuous vessels, ducts, and cavities found in the body as well as tissue tracts. Such closure devices and methods utilize the body's own natural healing mechanism to achieve hemostasis. This natural hemostatic process is further accelerated by the integration of bio-chemical agents or means for delivering such agents.

In a first aspect of this invention, a device for closing a blood vessel puncture site disposed at a distal end of a tissue tract comprises a shaft having a proximal end and a distal end, an expansible member, a bio-chemical sealing member, and a bio-chemical region or release region. The shaft is configured to advance through the tissue tract while the expansible member disposed on the distal end of the shaft is deployable within the blood vessel. The bio-chemical sealing member is slidably disposed over the shaft and proximal the expansible member. The bio-chemical region or release region is disposed under the sealing member. Advantageously, displacement of the bio-chemical sealing member in a proximal direction exposes the region so as to allow for safe and controlled release of bio-chemical agents into the tissue tract for enhanced and complete hemostasis of the puncture site.

The bio-chemical sealing member prevents severe complications as a result of bio-chemical agents from coming in contact with the blood stream by only allowing for the controlled exposure of such agents in the tissue tract. The sealing member has a length in a range from about 0.1 cm to about

100 cm, typically from about 5 cm to about 20 cm and a diameter in a range from about 0.5 mm to about 5 mm, typically from about 1 mm to about 3 mm. The sealing member may be a tubular member formed from a variety of medical grade materials, including coiled stainless steel tubing or polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like.

In a preferred embodiment of the device, a tensioning element, such as a spring or coil, is further provided. The tensioning element is slidably disposed over the shaft and under the sealing member proximal the expansible member. Generally, during application of the device, the tensioning element is preferably positionable in the tissue tract, but in other instances may be outside the tissue tract. The tensioning element gauges how much tension is being applied to the expansible member as it is seated against the puncture site so as to prevent a user from applying excessive force on the device causing undesirable movement (e.g., device is pulled out of patient body). The tensioning element also provides device compliance in cases of patient movement while the device is in place. The expansible member allows for sealing of the puncture site while the tensioning element along with an external clip apply and maintain tension to the expansible occluder so that it is seated against the puncture site at a vascular surface (e.g., blood vessel wall).

Positioning the expansible member against the vessel wall positions the bio-chemical region or release region outside the vessel lumen at a predetermined distance from the vessel wall and proximal the expansible member. Therefore, the expansible member provides not only occlusion at the vessel puncture site but also functions as a locator so as to position the bio-chemical region or release region outside the vessel lumen. This in turn ensures safe release of bio-chemical agents in the tissue tract and outside the blood stream. The predetermined distance is in a range from about 0 to about 20 mm, typically in a range from about 2 mm to about 10 mm.

The bio-chemical region or release region has a length in a range from about 1 mm to about 100 mm, typically in a range from about 5 mm to about 50 mm. It will be appreciated that the length and/or volume of the region may be varied in order to integrate and release the desired amount of bio-chemical agent. In one embodiment, the bio-chemical region includes at least one bio-chemical agent disposed on the distal end of the shaft proximal the expansible member and distal the tensioning element. In another embodiment, the region includes at least one bio-chemical agent disposed on the tensioning element. The agents may be coated, sprayed, molded, dipped, vapor deposited, plasma deposited, or painted thereon. Such a bio-chemical region on the occlusion device itself further minimizes variations due to user techniques, which may be particularly problematic with injection protocols where such agents are injected into the tract by the user. In yet another embodiment, the device may further incorporate an expansible feature disposed on the distal end of the shaft proximal the expansible member, wherein the region includes at least one bio-chemical agent associated with the expansible feature.

In alternative embodiments of the present invention, the device may further incorporate at least one bio-chemical delivery conduit disposed over the shaft and under the tensioning element and a bio-chemical injection port in fluid communication with the delivery conduit. The injection port may be connected to a syringe by use of a compression fitting or with an integrated luer lock. The bio-chemical agents are injected into the device via the syringe once the device is properly positioned. It will be appreciated that the size of the injection port and the delivery conduit may be selected to

control the delivery rate of such agents. In one example, the release region includes at least one opening, aperture, or orifice in fluid communication with a distal end of the conduit proximal the expansible member. It will be appreciated that any number, size, and/or shape of opening(s) may be utilized in order to obtain the desired release rate of bio-chemical agent. The release region may incorporate about 1 opening to about 100 openings, typically about 1 opening to about 10 openings. In another example, the release region includes at least one porous member in fluid communication with a distal end of the conduit proximal the expansible member so as to allow for the desired release of the bio-chemical agent.

A controlled delivery rate allows the bio-chemical agents to “ooze” out of the release region. This may eliminate the potential of high pressure release, which in turn minimizes the possibility of these agents from entering the blood stream. In addition, the sealing member serves to cover the bio-chemical release region so as to prevent any blood from flowing back through the release region, through the delivery conduit, and out through the injection port. The sealing member is only slidably displaced, revealing the bio-chemical release region, when it is desirable to deliver the bio-chemical agents.

The device of the present invention may further incorporate a spacer element disposed between the sealing member and the tensioning element so that the sealing member may easily slide over the tensioning element. The spacer element may be a tubular member formed from a variety of materials, including tubular polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like. The device further includes a handle on a proximal end of the shaft. A safety tab may be disposed between the handle and the sealing member. The safety tab prevents any undesirable displacement of the sealing member so as to inhibit inadvertent release of bio-chemical agents.

The present invention integrates the expansible member, bio-chemical sealing member, bio-chemical region or release region, and tensioning element in a single unitary catheter construction. This simple construction and user interface allows for safe, easy and convenient application of the device without numerous intermediary steps. The sealing member in combination with the locating expansible member ensures that the bio-chemical region or release region is only exposed in the tissue tract. This results in a more reliable, safe, and effective device which provides immediate and complete hemostasis, which in turn reduces the risk of bleeding, hematoma formation, thrombosis, embolization, and/or infection.

In another aspect of the present invention, methods for hemostasis of a puncture site in a blood vessel at a distal end of a tissue tract are provided. One method comprises introducing any one of the closure devices as described herein through the tissue tract. The expansible member is deployed at a distal end of the device within the blood vessel. The bio-chemical sealing member disposed proximal the expansible member is then displaced once properly positioned so as to expose a bio-chemical region or release region of the device. At least one bio-chemical agent is then released from the device and into the tissue tract.

The sealing member is displaced in a proximal direction so as to expose at least a portion of the region. This displacement distance is in a range from about 0.1 cm to about 10 cm, typically from about 0.5 cm to about 5 cm. The method further comprises deploying the tensioning element disposed proximal the expansible member within the tissue tract so that the expansible member is seated against a puncture site. Typically, deploying the tensioning element and displacing the

5

sealing member is carried out simultaneously so as to provide for easy and convenient application of the device without numerous intermediary steps. However, it will be appreciated that deployment of the tensioning element may be carried out independently, typically prior to displacement of the sealing member, so as to provide for proper positioning of the region or release region within the tissue tract and closure of the puncture site.

The amount of tension applied to the expansible member by the tensioning coil or spring is in the range from about 0.5 ounce to 30 ounces, typically in a range from about 2 ounces to 10 ounces. As described above, the expansible member locates and closes the puncture site in the blood vessel wall. Coil elongation is sufficient to provide adequate amount of tension on the expansible member to temporarily seal the puncture and to adequately displace the sealing member to reveal the bio-chemical region or release region. In some embodiments, coil elongation may be limited by a coupling member. Generally the amount of elongation of the tensioning coil may be the same as for displacement of the sealing member. The tension provided by the tensioning coil and the exposure of the bio-chemical agents may be maintained by application of an external clip on the tensioning coil, generally over the sealing member, wherein the clip rests over the skin at the puncture site.

Bio-chemical agent release generally comprises positioning the region at a predetermined distance proximal to the expansible member and outside the blood vessel wall. In particular, increasing the tension in the coil positions the expansible member against the puncture site and locates the bio-chemical region or release region in the tissue tract at the predetermined distance. Further increase in tension will cause the sealing member to disengage from an attachment point at the proximal end of the expansible member and the tensioning coil to elongate. Elongation of the tensioning coil will result in the sealing member to slide proximally so as to expose the region to the surrounding tissue for release of the bio-chemical agent.

The bio-chemical agents may accelerate the coagulation process and promote the formation of coagulum at the puncture site so to achieve complete hemostasis. The bio-chemical agent may comprise a variety of agents including clot promoting agents (e.g., thrombin, fibrinogen, etc.) or vaso-constricting agents (e.g., epinephrine, etc.). The bio-chemical agent is released for a time period in the range from about 0.1 minute to about 15 minutes, typically from about 0.5 minute to about 5 minutes. As described above, the occlusion device may be modified in several ways (e.g., region length, region volume, release region openings, conduit dimensions, number of conduits, or port dimensions) to achieve the desired bio-chemical agent release characteristics (e.g., rate, amount, time, etc.). The methods of the present invention may involve re-hydrating the bio-chemical agent with fluid in the tissue tract so as to generate coagulum. These agents may use the blood components to form a coagulum even at the presence of anti-coagulants.

As described above, the bio-chemical agent may be coated, sprayed, molded, painted, dipped, or deposited at the region. Alternatively, bio-chemical agents may be injected in a delivery conduit in fluid communication with at least one opening disposed at the release region. The sealing member in such an embodiment further prevents any blood from flowing back through the openings of the release region prior to placing the expansible member against the vessel wall when the release region is in the vessel lumen. Injection of bio-chemical agents in the presence of blood in the bio-chemical delivery pathway

6

may cause undesirable coagulum to form in the pathway which could prevent the bio-chemical agents from reaching the target site.

A further understanding of the nature and advantages of the present invention will become apparent by reference to the remaining portions of the specification and drawings.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The following drawings should be read with reference to the detailed description. Like numbers in different drawings refer to like elements. The drawings, which are not necessarily to scale, illustratively depict embodiments of the present invention and are not intended to limit the scope of the invention.

FIG. 1 illustrates a first embodiment of a drug eluting, self-tensioning vascular closure device for hemostasis of vascular puncture sites constructed in accordance with the principles of the present invention.

FIG. 2 illustrates an exploded view of the bio-chemical region on the distal end of the device of FIG. 1.

FIG. 3 illustrates the device of FIG. 1 in an expanded configuration with the occluding member deployed.

FIG. 4 illustrates the device of FIG. 1 in an expanded configuration with the occluding member under tension after removal of the safety seal and with the bio-chemical sealing member displaced proximally so as to expose the contents of the bio-chemical region.

FIGS. 5A through 5F illustrate a method for hemostasis of a puncture site in a body lumen employing the device of FIG. 1.

FIG. 6 illustrates a second embodiment of a drug eluting, self-tensioning vascular closure device for hemostasis of vascular puncture sites constructed in accordance with the principles of the present invention.

FIG. 7 illustrates an exploded view of the bio-chemical injection port and delivery conduit of the device of FIG. 6.

FIG. 8 illustrates an exploded view of the bio-chemical release region on the distal end of the device of FIG. 6.

FIG. 9 illustrates the device of FIG. 6 in an expanded configuration with the occluding member deployed.

FIG. 10 illustrates the device of FIG. 6 in an expanded configuration with the occluding member under tension and with the bio-chemical sealing member displaced proximally so as to expose the bio-chemical release region so that attachment of a syringe to the bio-chemical injection port provides delivery of bio-chemical agents.

#### DETAILED DESCRIPTION OF THE INVENTION

Referring now to FIG. 1, a first embodiment of a drug eluting, self-tensioning vascular occlusion device 70 for hemostasis of vascular puncture sites is illustrated, wherein at least one bio-chemical agent 152 is integrated with the device in a bio-chemical region or chamber 151. Device 70 generally comprises a first flexible elongated tubular member 71 formed from coiled stainless steel tubing or polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like. Tubular member 71 may have a length in a range from about 5 cm to about 50 cm, typically in the range from about 10 cm to about 30 cm and a diameter in the range from about 0.25 mm to about 5 mm, typically in the range from about 0.5 mm to about 2 mm. An expansible occlusion member 74 is disposed on the distal end of tubular member 71. A bio-chemical sealing member 153 is slidably disposed over the tubular member 71 and proximal the expansible member 74. The bio-chemical region 151 containing the

bio-chemical agent **152** is disposed under the sealing member **153**. It will be appreciated that the above depictions are for illustrative purposes only and do not necessarily reflect the actual shape, size, or dimensions of the device **70**. This applies to all depictions hereinafter.

The expansible member **74** may be formed from a variety of medical grade materials, including stainless steel, super-elastic material such as NITINOL®, or polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like. Preferably the expansible member **74** is made of superelastic NITINOL® material. The expansible member **74** in a retracted or collapsed state has a diameter of less than about 3 mm, preferably less than about 1.5 mm, as shown in FIGS. **1** and **2**. When deployed, the expansible member **74** in an expanded state has a diameter in a range from about 3 mm to about 20 mm, preferably from about 3.5 mm to about 8 mm, as shown in FIGS. **3** and **4**. Exemplary expansible structures **74** are described in detail in co-pending U.S. patent application Ser. No. 10/718,504. Still further embodiments of a braided mesh member **74** are described in U.S. Pat. No. 5,836,913.

The expansible member **74** may at least partially or preferably be fully covered with an elastomeric membrane material **96**. Membrane **96** may be formed from a variety of medical grade materials, such as thermoplastic elastomers (e.g., CHRONOPRENE® or POLYBLEND®) having durometers in a range from 15 Å to about 40 Å. Membrane **96** may be connected at a distal connection point **77** and a proximal connection point **75**. Adhesives such as LOCTITE® 4014 may be used to attach membrane **96** to the expansible member **74** and catheter shaft **71**. Alternatively, membrane **96** may take a form of a sock having its distal end sealed through a heat stake process or the like. In this case membrane **96** may not have to be attached distally. Membrane **96** preferably has a diameter that is sufficient to cover the expansible member **74**. In some embodiments, membrane **96** may be designed and attached to facilitate expansible member deployment as well as to reduce the amount of required elongation when the expansible member **74** is deployed. This may be achieved by molding the membrane **96** so that its midpoint diameter, where deployed expansible member **74** has its greatest diameter, is larger than its proximal and distal end diameters (e.g., a spherical shape). Membrane **96** may also be formed like a tube with a larger diameter than needed (e.g., diameter of retracted expansible member **74**), and then stretched over expansible member **74** and attached. The stretch should be enough to reduce the diameter of the membrane **96** to that of the expansible member **74**. In such a case, when member **74** is deployed, there is less elongation and stress experienced by membrane **96**. The membrane **96** may additionally form a membrane tip at a distal end of catheter **70** so as to provide a soft and blunt point for percutaneous access.

Referring now to FIG. **2**, the bio-chemical agents **152** may be composed of clot promoting agents such as thrombin and fibrinogen and/or vaso-constrictors such as epinephrine. These agents **152** may take on a form of a powder, paste that can be applied to the bio-chemical chamber or region **151**. Alternatively, such agents **152** may be molded in a form of a cylindrical tube with a longitudinal central hole that can be slidably disposed over member **71** and positioned between fixed attachment members **75** and **150** in the assembly process. The bio-chemical chamber/region **151** is located between the proximal end of member **75** and distal end of attachment member **150**. The length of region **151** determines the amount of bio-chemical agents **152** that can be integrated with the device, as well as the extent of the exposure of such agents to the tissue. It should also be noted that by increasing

the outside diameters of members **75** and **150**, the volume of chamber **151** can be increased and hence the volume of the bio-chemical agents **152** incorporated with the device.

The bio-chemical sealing member **153** generally comprises a flexible elongated tubular member. In a preferred embodiment, the tubular member **153** may have a length that extends from attachment member **75**, and overlapping member **75**, to grip member **85**, partially or fully overlapping member **85**. The inside diameter of member **153**, at least at the distal end, is similar to the outside diameter of member **75**. Member **153** is slidably positioned, at least partially, over member **75**. The interaction of members **153** and **75** provide for a fluid tight barrier so that blood will not come in contact with the bio-chemical agent prior to the intended time.

In the preferred embodiment of the present invention, a tensioning element **86** is slidably disposed over the tubular member **71** and proximal the expansible member **74**. the tensioning coil **86** is attached to the tubular member **71** with attachment member **150**. Member **150** may be in a tubular form and made from stainless steel tubing or polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like. Coil **86**, attachment member **150** and tubular member **71** are connected together by use of epoxy. The attachment point may be from 1 mm to 100 mm proximal to the member **75**, preferably in the range of 5 mm to 50 mm. The tensioning element **86** is described in more detail in co-pending U.S. patent application Ser. No. 10/974,008.

The function of bio-chemical seal **153** is to provide a barrier between the bio-chemical agents **152** and bodily fluids such as blood, and only allow the exposure of such agents to the tissue when the device is in correct position and the operator chooses to do so. Exposure of the bio-chemical region **151** to the surrounding tissue happens when the tensioning coil **86** is grabbed at grip member **85** and is pulled proximally with respect to member **75** to apply tension to the deployed expansible member **74** at the puncture site. The proximal pull of grip member **85** causes the tensioning coil **86** to elongate. The seal member **153** is attached to the coil **86** and grip member **85**. Since member **153** is not stretchable, the elongation of coil **86** results in disengagement of the distal end of member **153** from member **75**. Seal **153** slides proximally over the bio-chemical chamber/region **151** and exposes the bio-chemical agents **152** to the surrounding tissue. A spacer **154** provides adequate space between coil **86** and sealing member **153**, so that member **153** can easily slide over coil **86**. It should be noted that coil **86** elongation happens as the result of interference of the occluding expansible member **74** with the vessel wall at the puncture site. This in turn slides the sealing member **153** proximally, exposing the bio-chemical agents **152** in the tissue tract where it is needed.

It will be appreciated that bio-chemical seal **153** may be constructed to function independently from the tensioning coil **86**. Also, in some embodiments, a length of coil **86**, or the entire length of coil **86** may be coated with the bio-chemical agent **152**. In such case, when coil spring **86** is elongated to provide tension to the expansible member **74**, the deformation of the elongating coil spring **86** may result in breaking off of the agents **152** from the coil. This may result in faster re-hydration of the bio-chemical agents **152** and consequently acceleration of the coagulation process in the tract. Still further, the bio-chemical chamber **151** of device **70** may include an expansible feature over which the bio-chemical agent **152** is dispensed (e.g., coated). When desirable, this expansible member which may take the form of a balloon or a braided mesh, can be expanded, resulting in the agents **152** breaking off in the surrounding tissue, and hence accelerating the bio-chemical reaction.

The device 70 of the present invention may further incorporate a safety seal 155 to prevent inadvertent release of bio-chemical agents 152 by preventing coil 86 from sliding over member 71. Safety seal 155 may be made of different materials and be implemented in different fashions. One such implementation may take the form of heat shrinkable tubing. The tubing may be shrunk over member 71 to the proximal end of the coil 86 or preferably overlapping grip member 85. To remove the safety seal with ease, seal 155 may have a tab 156 that may be easily grabbed and pulled, tearing the safety seal 155 along the length of member 71. Removal of the safety seal 155 would allow coil 86 to freely slide over tubular member 71, exposing the bio-chemical agents 152 to the surrounding tissue.

The bio-chemical agent 152 is sealed from coming in contact with the circulating blood and generally is released in the tissue tract in the fascia at the puncture site. During device application, the expansible member 74 will be positioned and anchored against the puncture site in the vessel lumen. In particular, the expansible member 74 allows for sealing of the puncture site and locating the bio-chemical agents 152 appropriately in the tissue tract. The tensioning element 86 applies and maintains tension to the expansible occluder 74 while the sealing member 153 simultaneously reveals the bio-chemical agents 152 to bring such agents in contact with the surrounding tissue to accelerate the process of hemostasis.

Referring now to FIGS. 3 and 4, a proximal end of the device 70 comprises deployment means 78. Deployment of the expansible member 74 typically comprises pushing or pulling the two part handle assembly 78 coupled to the expansible member 74. A proximal end of handle assembly 78 comprises an actuating assembly 101 which is coupled to a push/pull member 76. Proximal movement of assembly 101 relative to a grip handle 102 deploys the expansible member 74. The grip handle 102 comprises a tubular member 103 formed from suitable metal tubing (e.g., stainless steel) or polymer materials (e.g., polyurethane, polyimide, PEEK®, PEBAX®, and the like). Member 103 is coupled to the catheter shaft 71 by means of an expander element 104 so as to account for the difference in an outside diameter of catheter 71 and an inside diameter of member 103. Elements 71, 103, and 104 may be attached by the use of adhesives. Member 103 further includes a feature 105, such as an indentation from a crimping process when element 103 is formed from a stainless steel or other metallic hypotube. Indentation 105 provides interference to element 106 of the actuating assembly 101.

Actuating assembly 101 further includes a tubular member 107 that is attached to the push/pull member 76 by a crimp process and/or adhesive. Member 107 provides added stiffness to the actuating mechanism 101 as well as provides for a larger surface area that consequently allows for enhanced adhesion of elements 106, 108, and 109 to member 107. These elements may comprise individual, separate parts, preferably formed from polymer materials such as polyurethane, polyimide, PEEK®, PEBAX®, and the like. These elements may be optionally incorporated into element 107 through an over molding process. Once the device 70 is deployed, interference of detent element 106 with indentation 105 securely maintains the expansible member 74 in its deployed position as shown in FIGS. 3 and 4. A proximal end of detent 106 may have a shallow angle in relation to the catheter shaft 71 so as to provide simplified deployment of the expansible member 74. A distal end of detent 106 may be more perpendicular to the catheter shaft 71 so as to provide more interference to feature 105, thereby requiring greater force to undeploy the expansible member 74. The increased

undeployment force is desirable to avoid inadvertent device collapse. Optionally, indentation 105 may be designed so that a distal side of the feature has a much shallower angle in relation to the catheter shaft 71 than a proximal side.

Elements 108 and 109 primarily provide support and alignment of the actuating assembly 101. Element 109 may be formed from a bright distinct color to indicate when the expansible member 74 is deployed. Element 110 comprises a tubular member, preferably having the same outer diameter as member 103. A distal end of tubular member 110 abuts a proximal end of member 103 so as to provide a positive stop to the movement of the actuating assembly 101 during the undeployment of the expansible member 74. Cap 111 at the most proximal end of the device 70 provides a soft tip for easier undeployment of expansible member 74. Cap 111 may be formed from rubber or similar materials.

In operation, handle assembly 78 is held by grabbing onto element 103 with one hand and element 110 with the other hand. Element 110 is then pulled in a proximal direction while holding element 103 stationary. As element 110 is pulled back, detent 106 slides over indentation 105 until it is completely moved to the proximal side of feature 105. FIGS. 3 and 4 illustrate the expansible member 74 that is in the form of a tubular braided mesh in the deployed and expanded state. The interference between elements 105 and 106 keeps the expansible member 74 in the deployed configuration. Undeployment of the device 70 may be effected with a single hand. In particular, member 103 may be grabbed by the palm of the hand while the thumb presses on cap 111. This causes the actuating mechanism 101 to move forward and the detent member 106 to slide distally over feature 105 resulting in the retraction of the expansible member 74.

Referring now to FIGS. 5A through 5F, a method for hemostasis of a puncture site in a body lumen employing the device 70 of FIG. 1 is illustrated. FIG. 5A depicts an existing introducer sheath 40 advanced through an opening in a skin surface 46, tissue tract in fascia 45 and vessel wall 43 and seated in a vessel lumen 41 at the completion of a catheterization procedure. Device 70 is then inserted through the hub of the sheath 40 and is advanced until the expansible member 74 is outside the sheath 40 and in the vessel lumen 41, as shown in FIG. 5B. This positioning may be indicated by a mark or feature on the catheter 71 or the handle assembly 78.

As shown in FIG. 5C, the expansible member 74 is then deployed by operation of the handle assembly 78. The sheath 40 is then slowly pulled out of the body, placing the expansible member 74 against the inner wall of the vessel 43 at the puncture site 42. As the sheath 40 is removed, the grip member 85 which is slidably disposed over the catheter shaft 71 and the handle assembly 78 are revealed. Sheath 40 is then discarded, leaving deployed expansible member 74 seated at the puncture site 42 and the bio-chemical chamber/region 151 in the tissue tract 47 as shown in FIG. 5D. If the device is equipped with the safety seal 155 as in device 70, then the safety seal 155 is removed by pulling the tab 156 proximally along the catheter shaft.

Referring now to FIG. 5E, once safety seal 155 is removed, the grip element 85 is grabbed and pulled in a proximal direction. Grip 85 is moved proximally to provide adequate amount of tension to the deployed expansible member 74 to achieve hemostasis. Typically, the amount of tension applied to the expansible member 74 is in the range of 0.5 ounces to 30 ounces. In particular, proximal movement of grip 85 causes simultaneous elongation of the tensioning coil 86, causing the expansible member to locate and close the puncture site 42, and displacement of the bio-chemical seal 153, exposing the bio-chemical agent 152 to the surrounding tis-

sue at a predetermined distance from the puncture site. The elongated position of coil **86** is maintained by application of a small external clip **50** to the catheter and seated against the surface of the skin **46**, as shown in FIG. **5E**. Device **70** is left in this position for a period of time to allow the bio-chemical agent **152** to reconstitute with the fluids in the tissue tract **47**, generating coagulum. Clip **50** is then removed and the expandible member **74** is collapsed by manipulation of the handle assembly **78**. Device **70** is then removed, leaving the active bio-chemical agents **152** and the coagulum in the tract **47** and adjacent the vessel puncture site **42**, as shown in FIG. **5F**. Additional finger pressure at the puncture site may be required to allow the coagulum to seal the small hole left in the vessel wall after removal of the device.

Referring now to FIG. **6**, another embodiment of an exemplary drug eluting, self-tensioning vascular occlusion device **80** for hemostasis of vascular puncture sites is illustrated, wherein the bio-active agents **152** may be stored separately and safely injected into the target site through a bio-chemical release region **163** once the device is properly positioned. The bio-chemical delivery system of device **80** is composed of an elongated tubular member **160**. Member **160** may be coaxially located over member **71** as shown in FIG. **6**. **160** has an inside diameter that is larger than the outside diameter of member **71**. Member **160** is formed from coiled stainless steel tubing or polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like. The gap made between the inside of member **160** and the outside of member **71** defines the bio-chemical delivery conduit **161**.

Referring now to FIG. **8**, the distal end of member **160** has a plurality of openings **162** defining the bio-chemical release region **163**. Openings **162** vary in number and may be from 1 opening to 100 opening, preferably from 1 opening to 10 openings. The size, shape, and/or number of openings **162** determines the rate of the release of the bio-chemical agents into the surrounding tissues. Alternatively, the bio-chemical release region **163** may not be part of member **160**, and may be a separate member, made of porous material which is in fluid communication with member **160**. In either embodiment, release region **163** is located at a predetermined distance proximal to the expandible member **74**.

Referring now to FIG. **7**, a bio-chemical injection port **164** is illustrated. Port **164** comprises a flexible elongated tubular member that transitions to member **160** at its distal end by means of a coupling member **165**. At a proximal end, the port **164** provides a coupling to a syringe **167** for the injection of bio-chemical agents **152**. Members **164** and **165** may be constructed from stainless steel tubing or polymer materials such as nylon, polyurethane, polyimide, PEEK®, PEBAX®, and the like. Member **165** may or may not be a flexible member. Member **165** preferably has an outside diameter that is not larger than the outside diameter of the handle assembly **78**. This ensures that device **80** can go through the existing sheath **40** without interference, as was described for device **70** in FIGS. **5A** through **5F**. Coupling member **165** is connected to member **160** via member **166**. Members **164**, **165** and **160** are attached by means of epoxy to provide a fluid tight seal at attachment points **166**.

It will be appreciated that the drug delivery conduit **160** may comprise a single or multiple elongated tubular member (s) of varying length(s) that run(s) along the length of member **71**. At a proximal end, these conduits couple into delivery port **164** via coupling member **165**. At a distal end, these tubular members may terminate at different points proximal to the expandible member **74**, dispersed over release region **163**. Distally, these conduits may have at least one opening for the release of the bio-chemical agents into the region.

The bio-chemical sealing member **153** of device **80** functions in a similar fashion as in device **70**. In addition, the sealing member **153** of device **80** prevents blood from flowing back through the bio-chemical deliver path **163**, **162**, **161**, **164**. However, it will be appreciated that the back flow of blood through the bio-chemical delivery pathway may be used as an indicator that the bio-chemical release region **163** is in the vessel lumen. When the back flow stops, that may be an indication that the release region **163** is in the tissue tract, where there is no appreciable blood pressure. In addition to the expandible member **74**, this feature may add more certainty to the positioning of the bio-chemical release region **163** and hence improve safety. In such case, prior to injection of the bio-chemical agents **152**, the pathway may be flushed with solutions such as saline.

The tensioning coil **86**, spacer element **154**, and grip member **85** of device **80** function in a similar fashion as in device **70**. In device **80**, however, the elongation of tensioning coil **86** is limited by the distal end of coupling member **165** at attachment point **166**. The distance between the proximal end of the coil spring **86** and the distal end of coupling member **165** at point **166** is long enough to provide the adequate amount of tension. This distance is also sufficient to allow the bio-chemical seal **153** to move proximally to expose the entire bio-chemical release region **163**. FIG. **9** illustrates device **80** with a deployed expandible member **74**. FIG. **10** illustrates device **80** when the coil **86** is elongated to apply adequate amount of tension to expandible member **74** and to expose the bio-chemical release region **163**. The attachment of syringe **167** to delivery port **164** for delivery of bio-chemical agents **152** to the target site is also illustrated.

In operation, device **80** is inserted through the sheath **40** and advanced until the expandible member **74** is out of the sheath **40** and in the blood vessel **41**. The expandible member **74** is deployed by manipulation of the handle assembly **78**, the sheath **40** is removed and discarded, and the deployed expandible member **74** is placed against the inside wall of the vessel at the puncture site **42**. Tension is then applied by proximally sliding grip member **85** of coil **86**. The applied tension at the deployed expandible member **74** will provide hemostasis, and locates bio-chemical release region **163**. Elongation of the coil **86** reveals the bio-chemical release region **163** to the surrounding tissue tract **47**. The tension and coil elongation are maintained by application of an external clip **50**. Syringe **167** containing the bio-chemical agents **152** is then connected to the bio-chemical injection port **164**. An adequate amount of the agent(s) is injected into the site at tissue tract **47**. The bio-chemical agents **152** promote and accelerate the hemostatic process. After injection of the bio-chemical agents **152**, enough time is given for the agents to react with the blood tissue to form coagulum. External clip **50** is then removed, expandible member **74** is collapsed, and device **80** is removed. Removal of the device **80** may be followed by a few minutes of manual compression at the site to close the small hole left in the vessel wall.

Although certain exemplary embodiments and methods have been described in some detail, for clarity of understanding and by way of example, it will be apparent from the foregoing disclosure to those skilled in the art that variations, modifications, changes, and adaptations of such embodiments and methods may be made without departing from the true spirit and scope of the invention. Therefore, the above description should not be taken as limiting the scope of the invention which is defined by the appended claims.

What is claimed is:

1. A method for closing a blood vessel puncture site disposed at a distal end of a tissue tract, the method comprising:

## 13

introducing a closure device through the tissue tract, wherein a bio-chemical agent region of the closure device is coated with at least one bio-chemical agent prior to being introduced through the tissue tract;

5 deploying an expansible member at a distal end of the device within the blood vessel after the closure device, including the bio-chemical agent region, has been introduced through the tissue tract; and

10 displacing a bio-chemical region sealing member disposed proximal the expansible member so as to both expose the bio-chemical agent coated on the bio-chemical agent region of the device and apply tension to the expansible member through a tensioning element of the closure device to seat the expansible member against a puncture site; and

15 wherein the at least one bio-chemical agent hydrates into surrounding fluids to form a coagulum in the tissue tract, wherein the tensioning element is disposed proximal the expansible member and is disposed coaxially over and surrounding an inner shaft of the closure device so that the expansible member is seated against a puncture site.

2. The method of claim 1, wherein the sealing member is displaced a distance in a range from about 0.1 cm to about 10 cm.

25 3. The method of claim 1, wherein deploying the tensioning element and displacing the sealing member is carried out simultaneously or sequentially.

4. The method of claim 1, further comprising limiting elongation of the tensioning element.

30 5. The method of claim 1, further comprising locating and closing the puncture site in the blood vessel wall with the expansible member.

6. The method of claim 5, further comprising positioning the region at a predetermined distance proximal to the expansible member and blood vessel wall.

35 7. The method of claim 1, wherein the bio-chemical agent comprises a clot promoting or vaso-constricting agent.

8. The method of claim 7, wherein the bio-chemical agent is released for a time period in the range from about 0.1 minute to about 15 minutes.

40 9. The method of claim 1, wherein the bio-chemical agent consists essentially of thrombin or fibrinogen.

## 14

10. The method of claim 1, wherein the bio-chemical agent is released over a time from 0.1 minute to 15 minutes.

11. The method of claim 1, further comprising withdrawing the closure device, including the bio-chemical agent region, from the tissue tract to leave in the tissue tract the at least one bio-chemical agent that has hydrated into surrounding fluids and coagulum generated from the at least one bio-chemical agent reconstituted with fluids in the tissue tract.

12. The method of claim 1, wherein the inner shaft of the closure device comprises a distal end coupled to the expansible member.

13. The method of claim 1, wherein the tensioning element comprises a coil spring.

14. The method of claim 1, wherein the tensioning element is disposed under the sealing member and proximal the expansible member.

15. The method of claim 1, wherein the tensioning element comprises a proximal end attached to a proximal end of the sealing member.

20 16. A method for closing a blood vessel puncture site disposed at a distal end of a tissue tract, the method comprising:

introducing a closure device through the tissue tract, wherein a bio-chemical agent region of the closure device is coated with at least one bio-chemical agent prior to being introduced through the tissue tract;

25 deploying an expansible member at a distal end of the device within the blood vessel after the closure device, including the bio-chemical agent region, has been introduced through the tissue tract; and

30 displacing a bio-chemical region sealing member disposed proximal the expansible member so as to both expose the bio-chemical agent coated on the bio-chemical agent region of the device and apply tension to the expansible member through a tensioning element of the closure device to seat the expansible member against a puncture site; and

35 wherein the at least one bio-chemical agent hydrates into surrounding fluids to form a coagulum in the tissue tract, and

40 wherein the tensioning element comprises a coil spring.

\* \* \* \* \*