



US008834538B2

(12) **United States Patent**  
**Donnelly et al.**

(10) **Patent No.:** **US 8,834,538 B2**  
(45) **Date of Patent:** **\*Sep. 16, 2014**

(54) **METHOD OF PERFORMING ANTERIOR CRUCIATE LIGAMENT RECONSTRUCTION USING BIODEGRADABLE INTERFERENCE SCREW**

(58) **Field of Classification Search**  
USPC ..... 606/300, 301, 304, 321, 323, 331, 88, 606/104, 77; 623/13.12, 13.11, 13.14, 623/13.13, 13.18  
See application file for complete search history.

(75) Inventors: **Lisa M. Donnelly**, Wayland, MA (US); **Yufu Li**, Bridgewater, NJ (US); **Joan M. Sullivan**, Hanover, MA (US); **Gregory R. Whittaker**, Stoneham, MA (US); **J. Jenny Yuan**, Neshanic Station, NJ (US)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,356,572	A	11/1982	Guillemin et al.
4,643,734	A	2/1987	Lin
4,645,503	A	2/1987	Lin et al.
4,655,777	A	4/1987	Dunn et al.
4,781,183	A	11/1988	Casey et al.
4,950,270	A	8/1990	Bowman et al.
5,108,755	A	4/1992	Daniels et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE	2742128	A1	3/1978
EP	0615732	A1	9/1994

(Continued)

OTHER PUBLICATIONS

EP Search Report dated Feb. 15, 2005 for EP Appl. No. 04 25 5926.

(Continued)

*Primary Examiner* — Pedro Philogene  
*Assistant Examiner* — David Comstock

(57) **ABSTRACT**

A method of replacing an ACL with a graft. The method provides for the drilling bone tunnels in a femur and a tibia. A replacement graft is provided having first and second ends. A biodegradable composite screw is provided. The screw is made from a biodegradable polymer and a bioceramic or a bioglass. At least one end of the graft is secured in a bone tunnel using the biodegradable composite screw.

**11 Claims, 15 Drawing Sheets**

(73) Assignee: **DePuy Mitek, LLC**, Raynham, MA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 376 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **13/191,078**

(22) Filed: **Jul. 26, 2011**


(65) **Prior Publication Data**  
US 2011/0282450 A1 Nov. 17, 2011

**Related U.S. Application Data**

(63) Continuation of application No. 10/673,737, filed on Sep. 29, 2003, now Pat. No. 8,016,865.

(51) **Int. Cl.**  
**A61B 17/86** (2006.01)  
**A61L 31/14** (2006.01)  
**A61L 31/12** (2006.01)

(52) **U.S. Cl.**  
CPC ..... **A61L 31/127** (2013.01); **A61L 31/148** (2013.01); **A61L 31/128** (2013.01)  
USPC ..... **606/301**

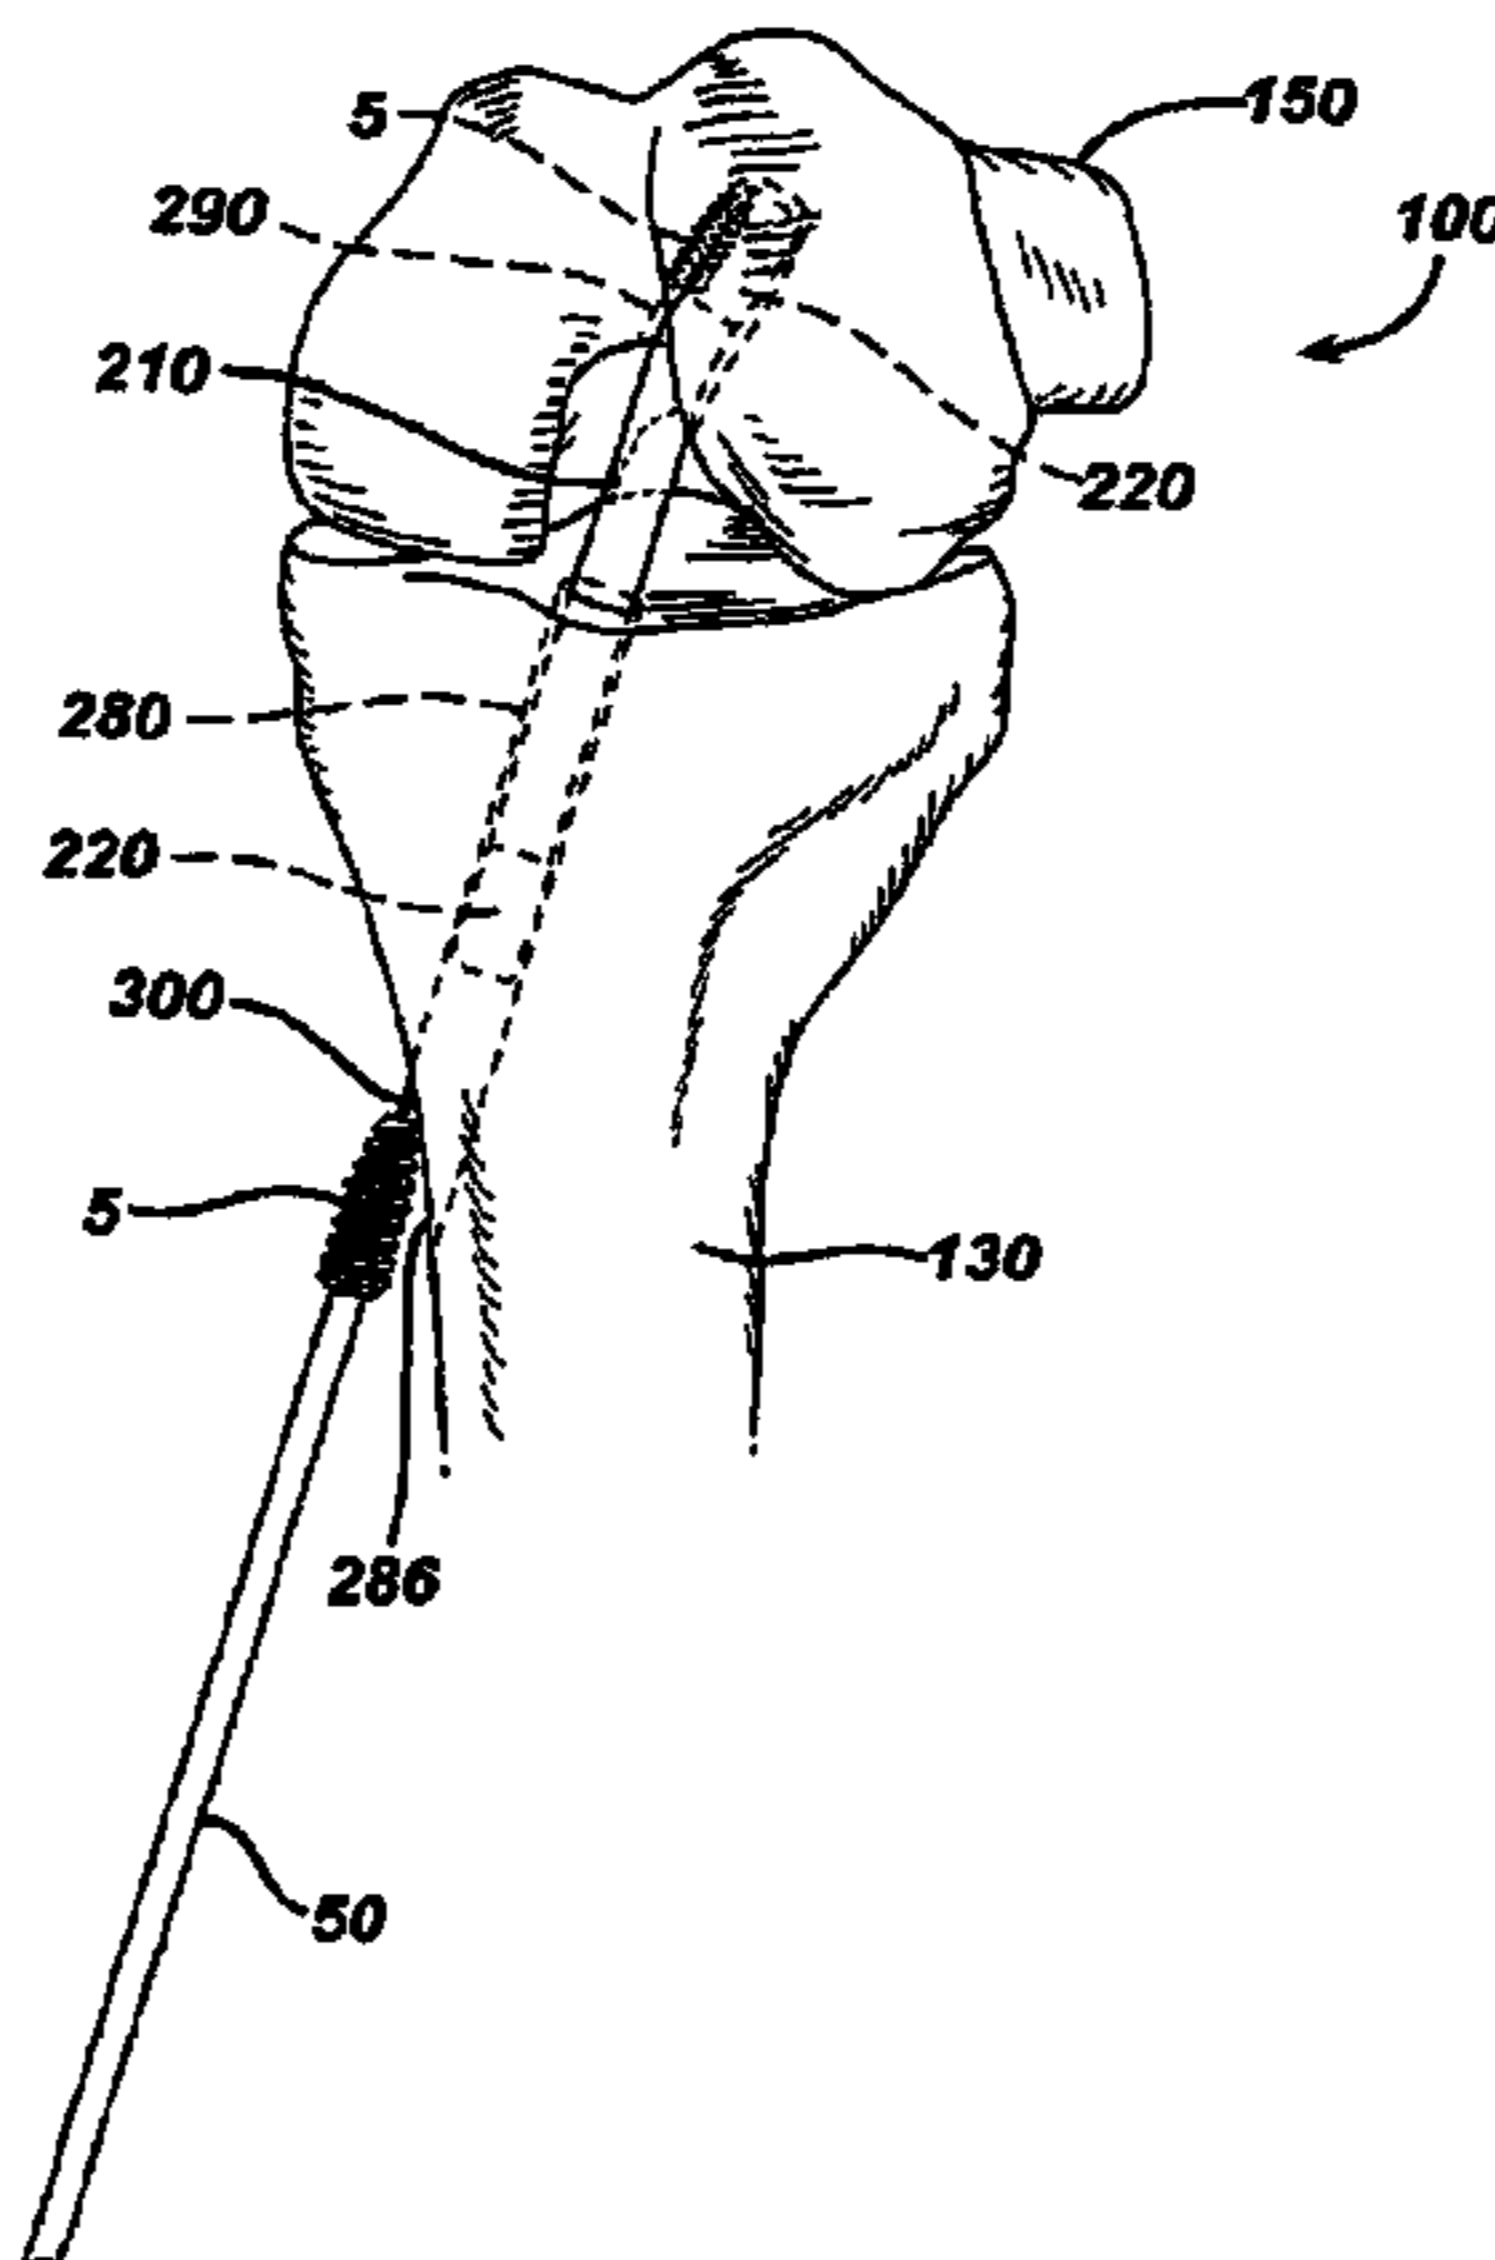

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,116,337 A 5/1992 Johnson  
 5,139,520 A 8/1992 Rosenberg  
 5,275,601 A 1/1994 Gogolewski et al.  
 5,364,400 A 11/1994 Rego, Jr. et al.  
 5,478,355 A 12/1995 Muth et al.  
 5,509,913 A 4/1996 Yeo  
 5,552,454 A 9/1996 Kretschmann et al.  
 5,584,836 A 12/1996 Ballintyn et al.  
 5,603,716 A 2/1997 Morgan et al.  
 5,618,314 A 4/1997 Harwin et al.  
 5,626,612 A 5/1997 Bartlett  
 5,632,748 A 5/1997 Beck, Jr. et al.  
 5,679,723 A 10/1997 Cooper et al.  
 5,681,873 A 10/1997 Norton et al.  
 5,716,359 A 2/1998 Ojima et al.  
 5,725,541 A 3/1998 Anspach, III et al.  
 5,741,329 A 4/1998 Agrawal et al.  
 5,747,390 A 5/1998 Cooper et al.  
 5,766,618 A 6/1998 Laurencin et al.  
 5,849,013 A 12/1998 Whittaker et al.  
 5,868,749 A 2/1999 Reed  
 5,871,504 A 2/1999 Eaton et al.  
 5,879,372 A 3/1999 Bartlett  
 5,955,529 A 9/1999 Imai et al.  
 5,962,007 A 10/1999 Cooper et al.  
 5,968,047 A 10/1999 Reed  
 5,971,987 A 10/1999 Huxel et al.  
 5,977,204 A 11/1999 Boyan et al.  
 5,980,252 A 11/1999 Samchukov et al.  
 5,980,574 A 11/1999 Takei et al.  
 6,001,100 A 12/1999 Sherman et al.  
 6,165,203 A 12/2000 Krebs  
 6,165,486 A 12/2000 Marra et al.  
 6,214,007 B1 4/2001 Anderson  
 6,254,562 B1 7/2001 Fouere  
 6,283,973 B1 9/2001 Hubbard et al.  
 6,325,804 B1 12/2001 Wenstrom, Jr. et al.  
 6,331,313 B1 12/2001 Wong et al.  
 6,402,766 B2 6/2002 Bowman et al.  
 6,406,498 B1 6/2002 Tormala et al.  
 6,471,707 B1 10/2002 Miller et al.  
 6,562,071 B2 5/2003 Jarvinen  
 6,565,573 B1 5/2003 Ferrante et al.  
 6,749,620 B2 6/2004 Bartlett  
 6,773,436 B2 8/2004 Donnelly et al.  
 6,866,666 B1 3/2005 Sinnott et al.  
 6,916,321 B2 7/2005 TenHuisen et al.  
 7,012,106 B2 3/2006 Yuan et al.  
 8,016,865 B2 9/2011 Donnelly et al.  
 2001/0007074 A1 7/2001 Strobel et al.  
 2001/0041937 A1 11/2001 Rieser et al.  
 2002/0072797 A1 6/2002 Hays et al.  
 2002/0099411 A1 7/2002 Bartlett  
 2002/0147463 A1 10/2002 Martinek  
 2002/0161371 A1 10/2002 Bezemer et al.  
 2003/0006533 A1 1/2003 Shikinami et al.  
 2003/0009235 A1 1/2003 Manrique et al.  
 2003/0026675 A1 2/2003 McGovern et al.  
 2003/0040695 A1 2/2003 Zhao et al.  
 2003/0065331 A1 4/2003 Donnelly et al.

2003/0074002 A1 4/2003 West  
 2003/0074004 A1 4/2003 Reed  
 2003/0105471 A1 6/2003 Schlapfer et al.  
 2003/0125744 A1 7/2003 Contiliano et al.  
 2003/0125749 A1 7/2003 Yuan et al.  
 2003/0233095 A1 12/2003 Urbanski et al.  
 2004/0001890 A1 1/2004 Rosenblatt et al.  
 2004/0006346 A1 1/2004 Holmen et al.  
 2004/0153075 A1 8/2004 Roger  
 2004/0181257 A1 9/2004 Bartlett  
 2004/0193285 A1 9/2004 Roller et al.  
 2004/0243178 A1 12/2004 Haut et al.  
 2004/0243180 A1 12/2004 Donnelly et al.  
 2005/0216016 A1 9/2005 Contiliano et al.  
 2005/0222618 A1 10/2005 Dreyfuss et al.  
 2005/0222619 A1 10/2005 Dreyfuss et al.  
 2005/0267479 A1 12/2005 Morgan et al.  
 2006/0015108 A1 1/2006 Bonutti  
 2006/0020266 A1 1/2006 Cooper  
 2006/0122624 A1 6/2006 Truckai et al.  
 2006/0149266 A1 7/2006 Cordasco  
 2006/0178748 A1 8/2006 Dinger et al.  
 2006/0229671 A1 10/2006 Steiner et al.  
 2006/0264531 A1 11/2006 Zhao  
 2007/0093895 A1 4/2007 Donnelly et al.


## FOREIGN PATENT DOCUMENTS

EP 0714666 A1 6/1996  
 JP 2002-035018 A 2/2002  
 JP 2003-506158 T 2/2003  
 JP 2003-180816 A 7/2003  
 WO WO-9001342 A1 2/1990  
 WO WO-9600592 1/1996  
 WO WO-0001426 A1 1/2000  
 WO WO-2003/011343 A1 2/2003


## OTHER PUBLICATIONS

Fink et al., "Bioabsorbable Polyglyconate Interference Screw Fixation in Anterior Cruciate Ligament Reconstruction: A Prospective Computed Tomology-Controlled Study," *Arthroscopy: The Journal of Arthroscopic and Related Surgery*, vol. 16, No. 5 Jul.-Aug., 2000: pp. 491-498.  
 J.L. Leray, "Biodegradable Composite Materials for Bone Surgery," *Trans. Soc. Biomater.*, 1, 70 (1977).  
 Office Action dated Aug. 16, 2005 in U.S. Appl. No. 10/673,737.  
 Office Action dated Dec. 31, 2007 in U.S. Appl. No. 10/673,737.  
 Office Action dated Feb. 19, 2010 in U.S. Appl. No. 10/673,737.  
 Office Action dated Feb. 23, 2006 in U.S. Appl. No. 10/673,737.  
 Office Action dated Jan. 26, 2005 in U.S. Appl. No. 10/673,737.  
 Office Action dated Jun. 1, 2007 in U.S. Appl. No. 10/673,737.  
 Office Action dated May 28, 2009 in U.S. Appl. No. 10/673,737.  
 Office Action dated Sep. 18, 2008 in U.S. App. No. 11/604,427.  
 Weiler et al., "Biodegradable Implants in Sports Medicine: The Biological Base," *Arthroscopy: The Journal of Arthroscopic and Related Surgery*, vol. 16, No. 3 (Apr. 2000): pp. 305-321.  
 Smith et al., "Fracture of Bilok Interference Screws on Insertion During Anterior Cruciate Ligament Reconstruction," *Arthroscopy: The Journal of Arthroscopic and Related Surgery*, vol. 19, No. 9 (Nov. 2003): e115-e117.

**FIG. 1A**

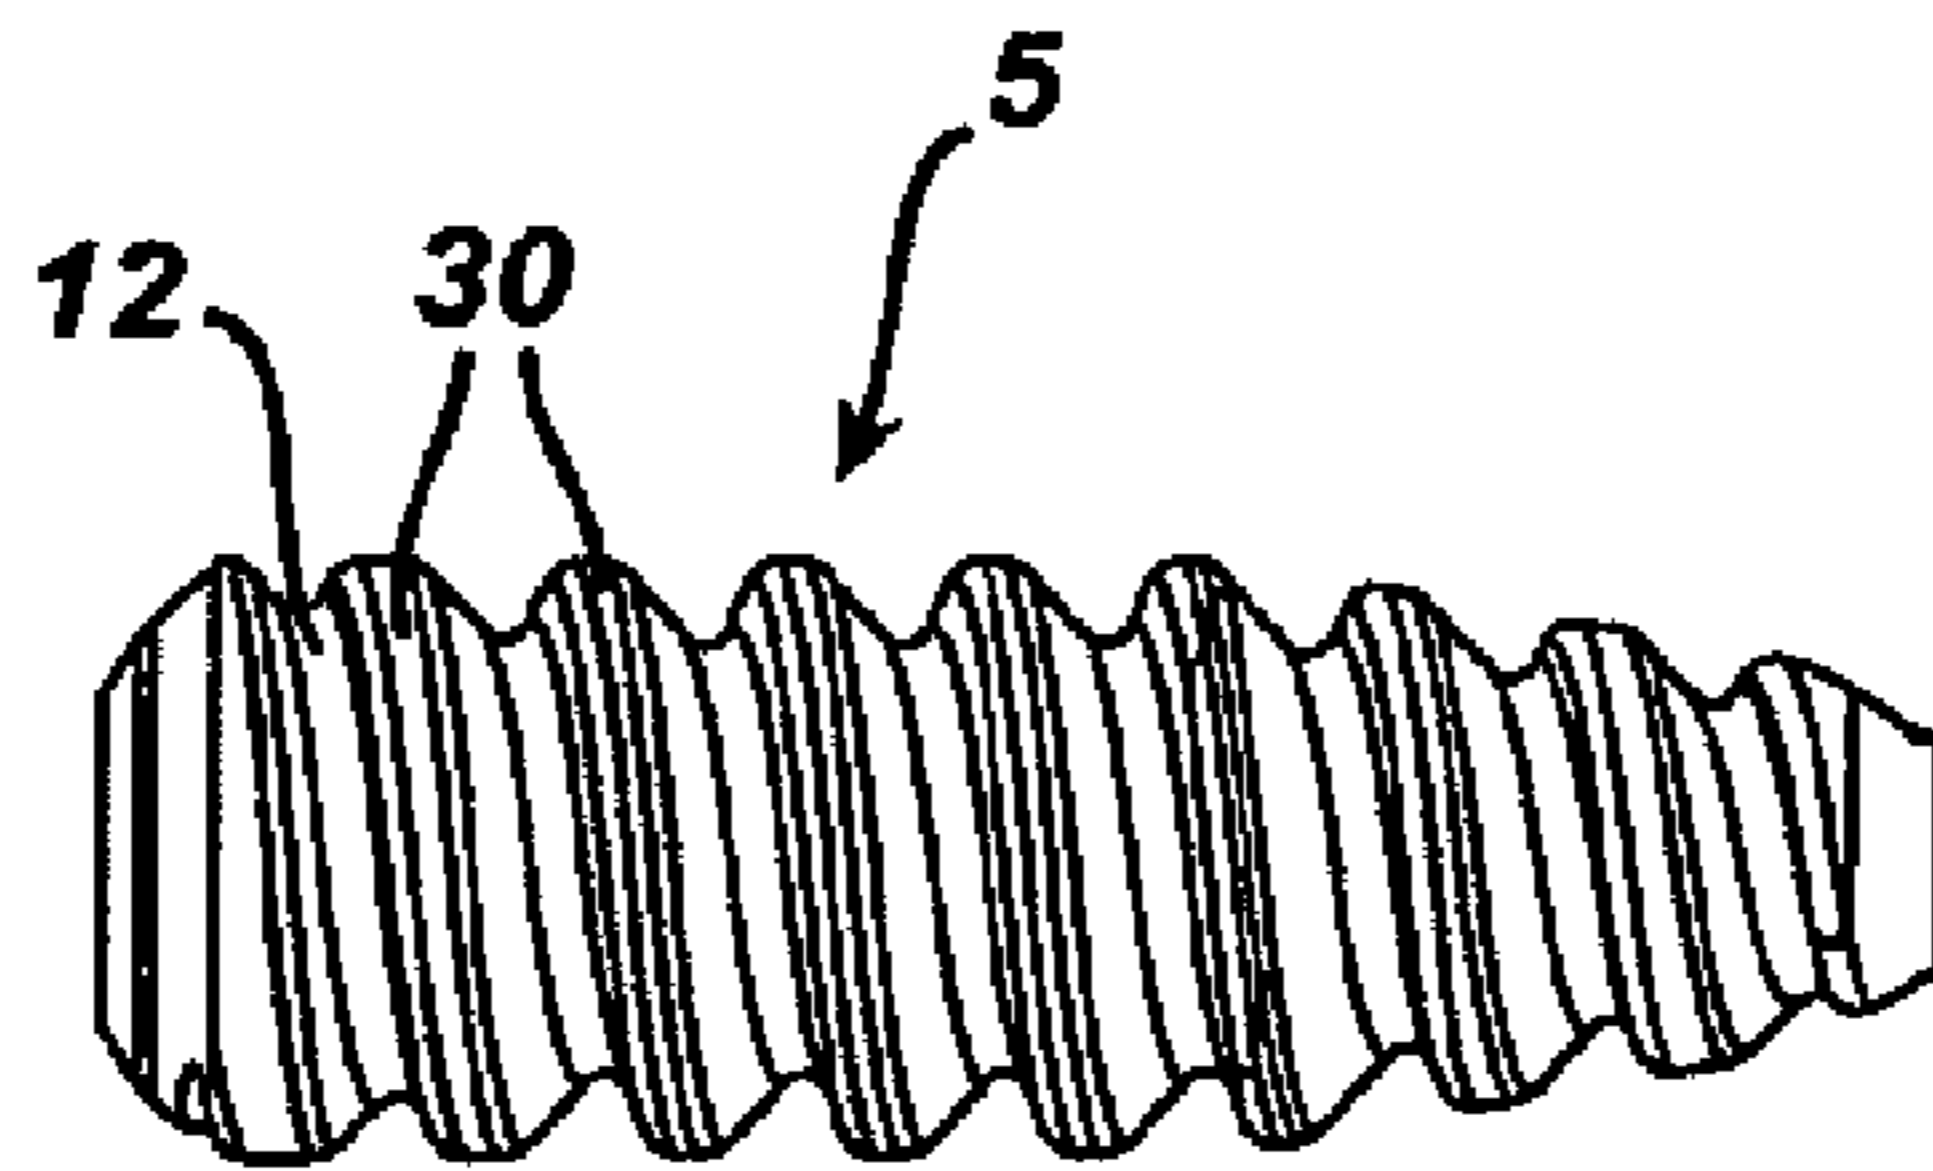

**FIG. 1B**

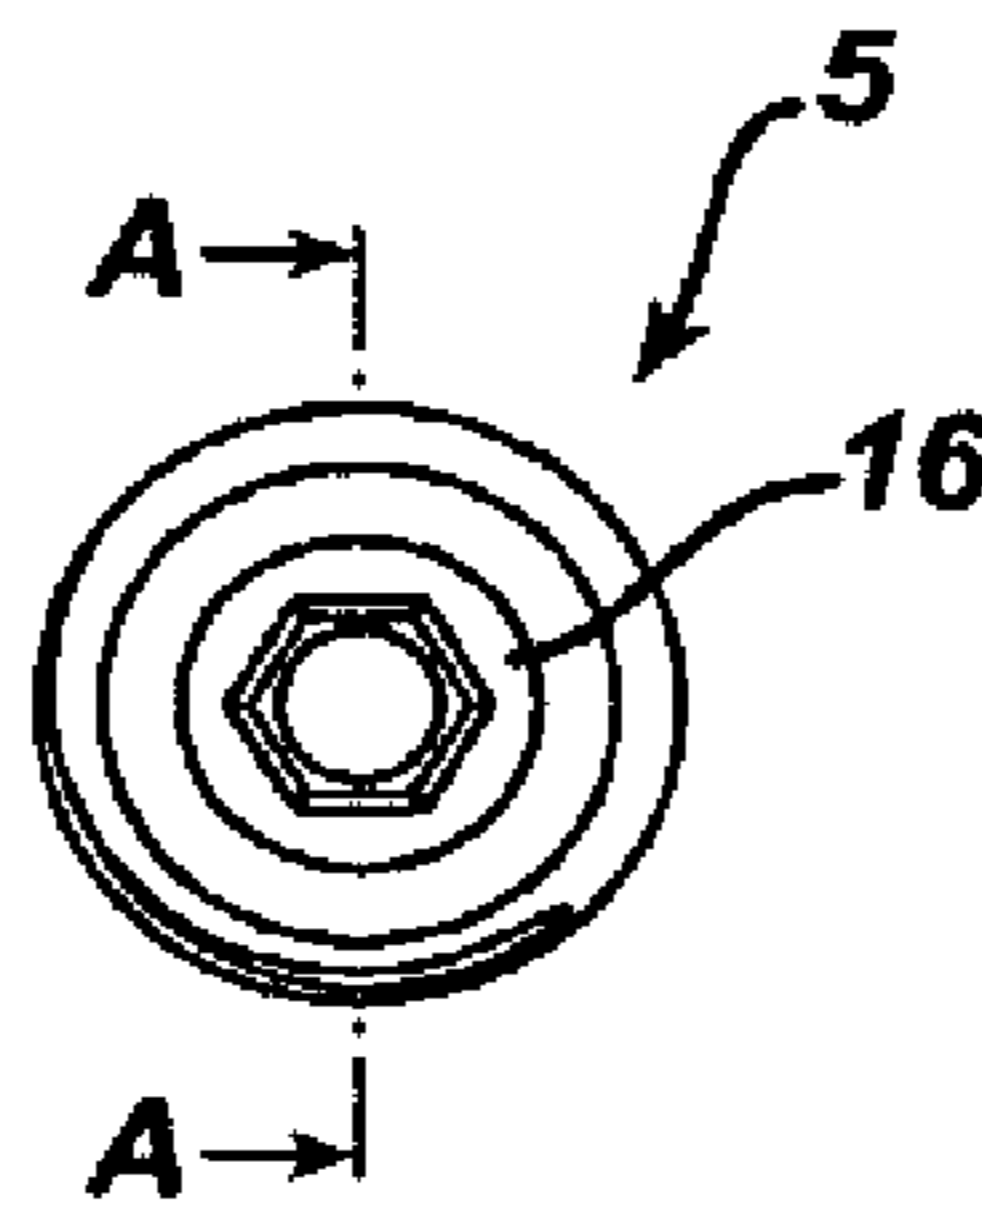

**FIG. 1C**



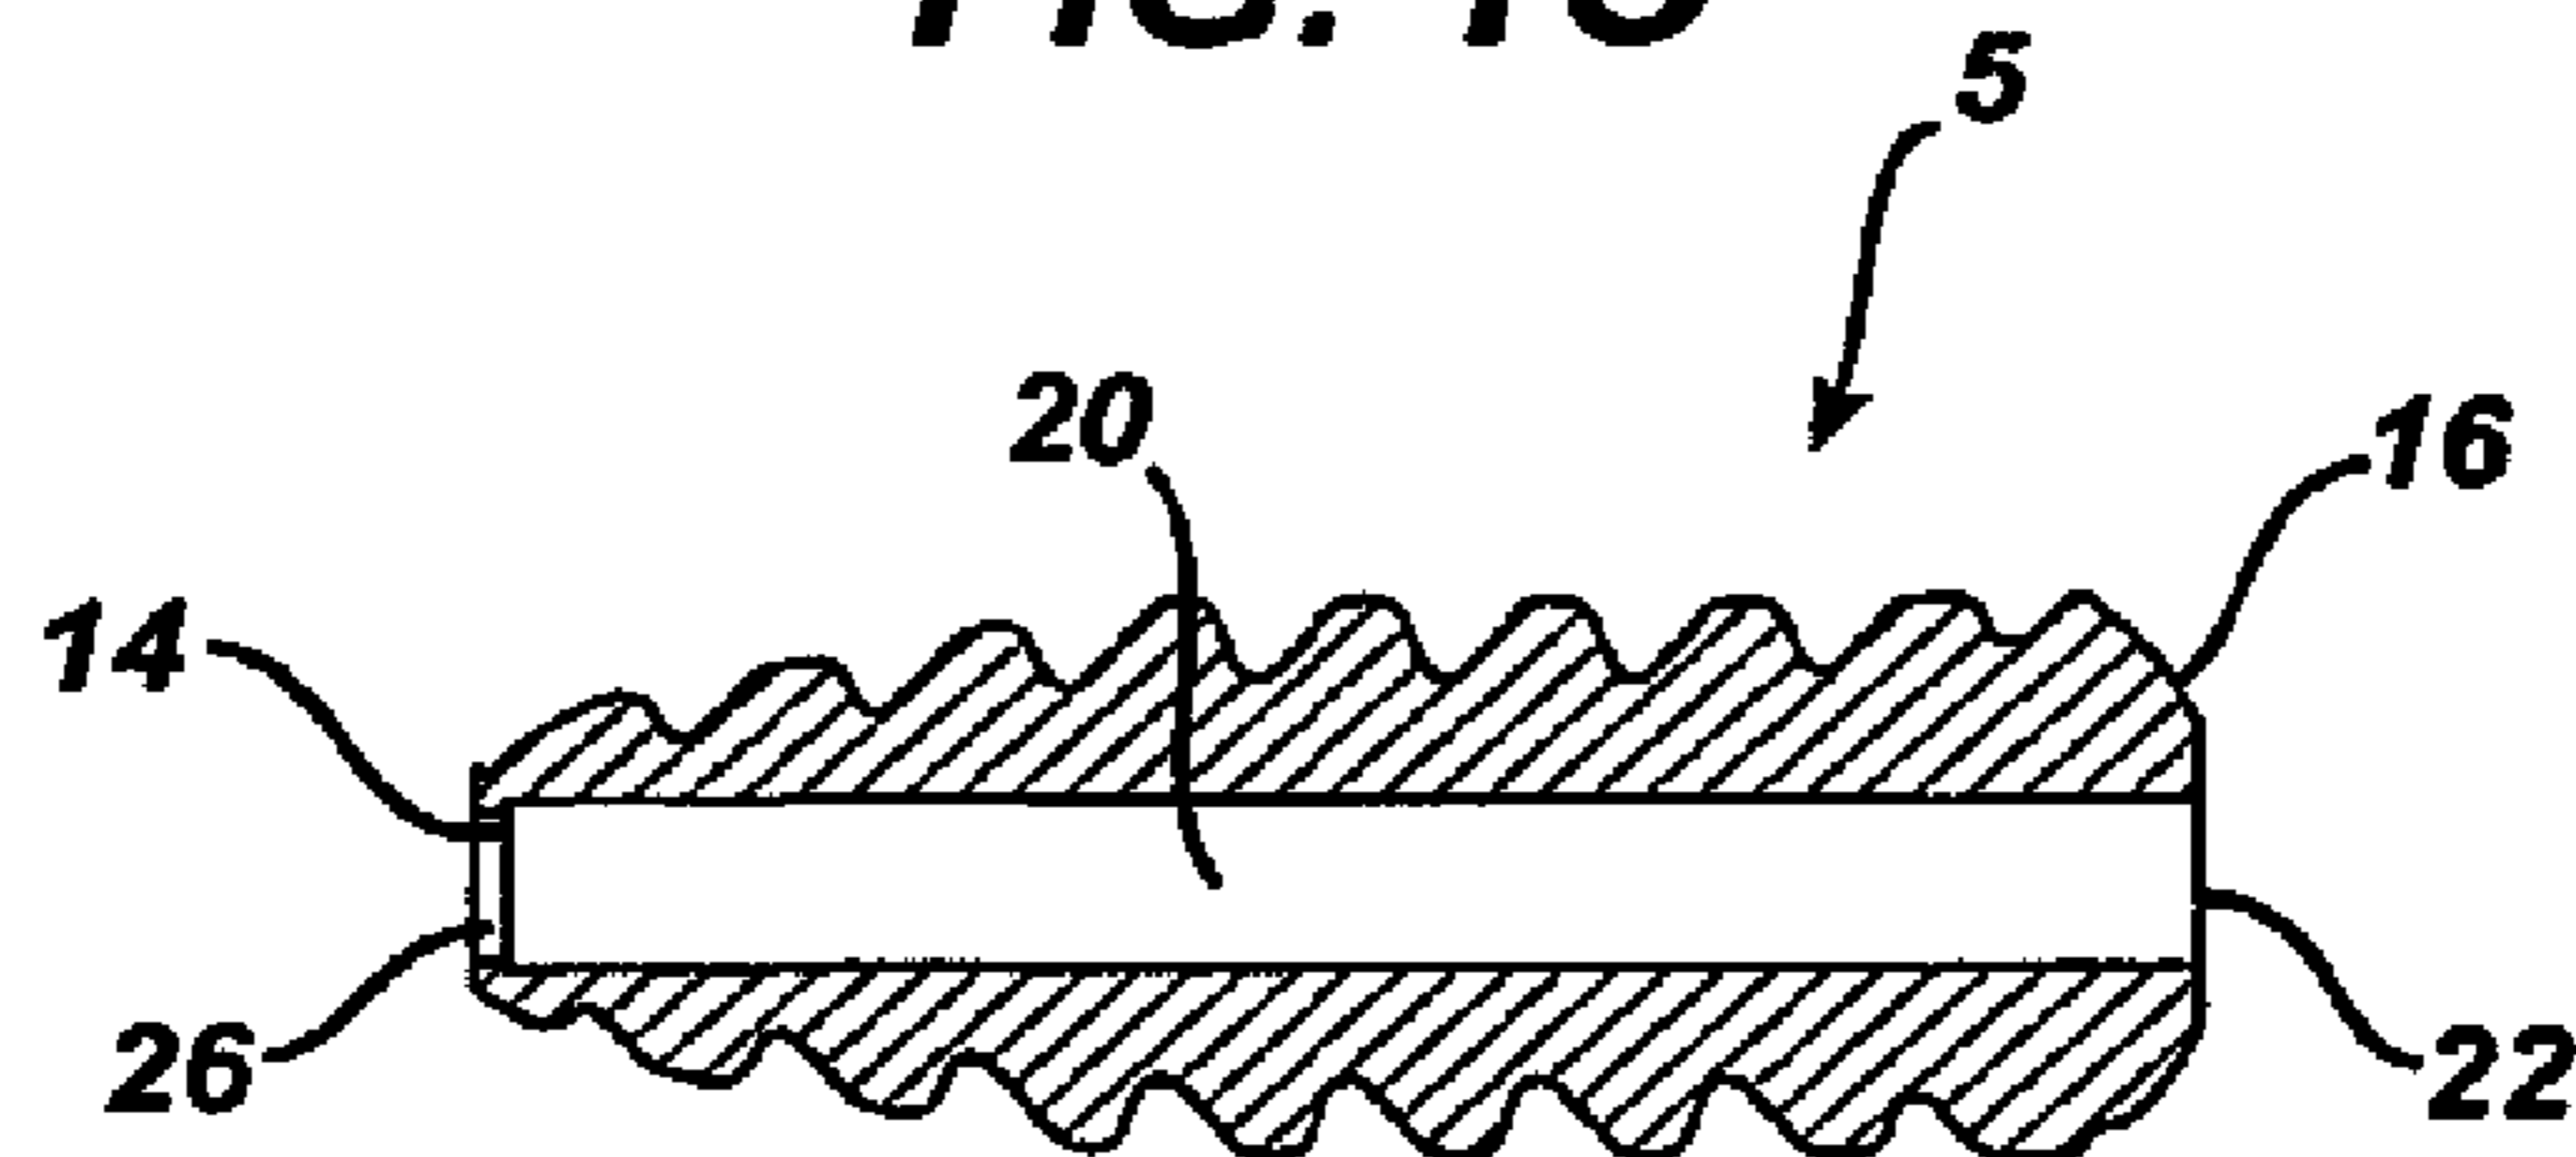





FIG. 2

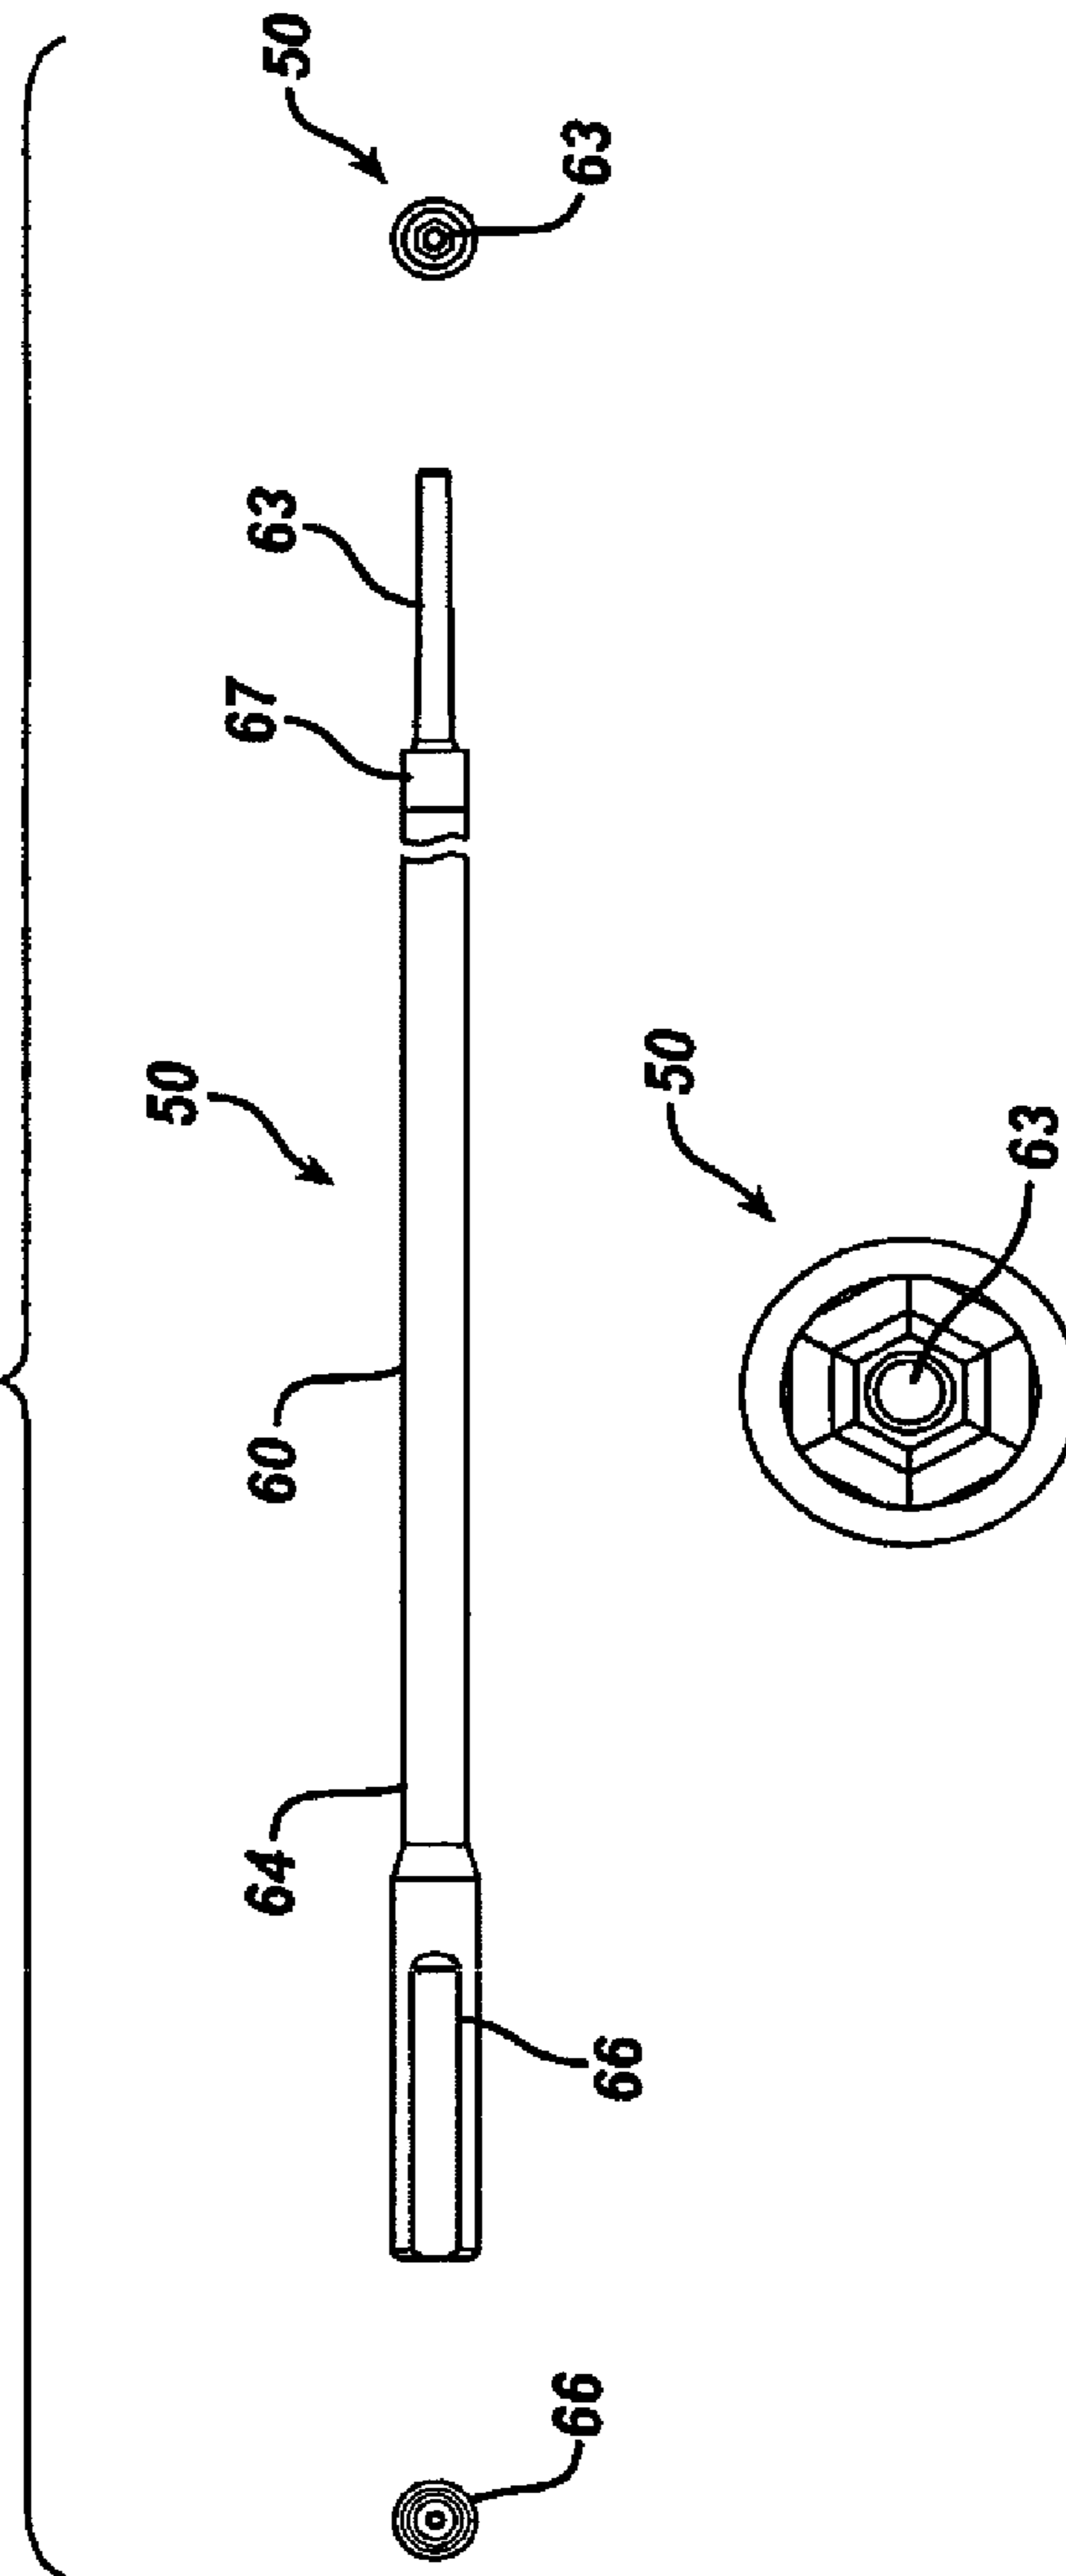


**FIG. 3**

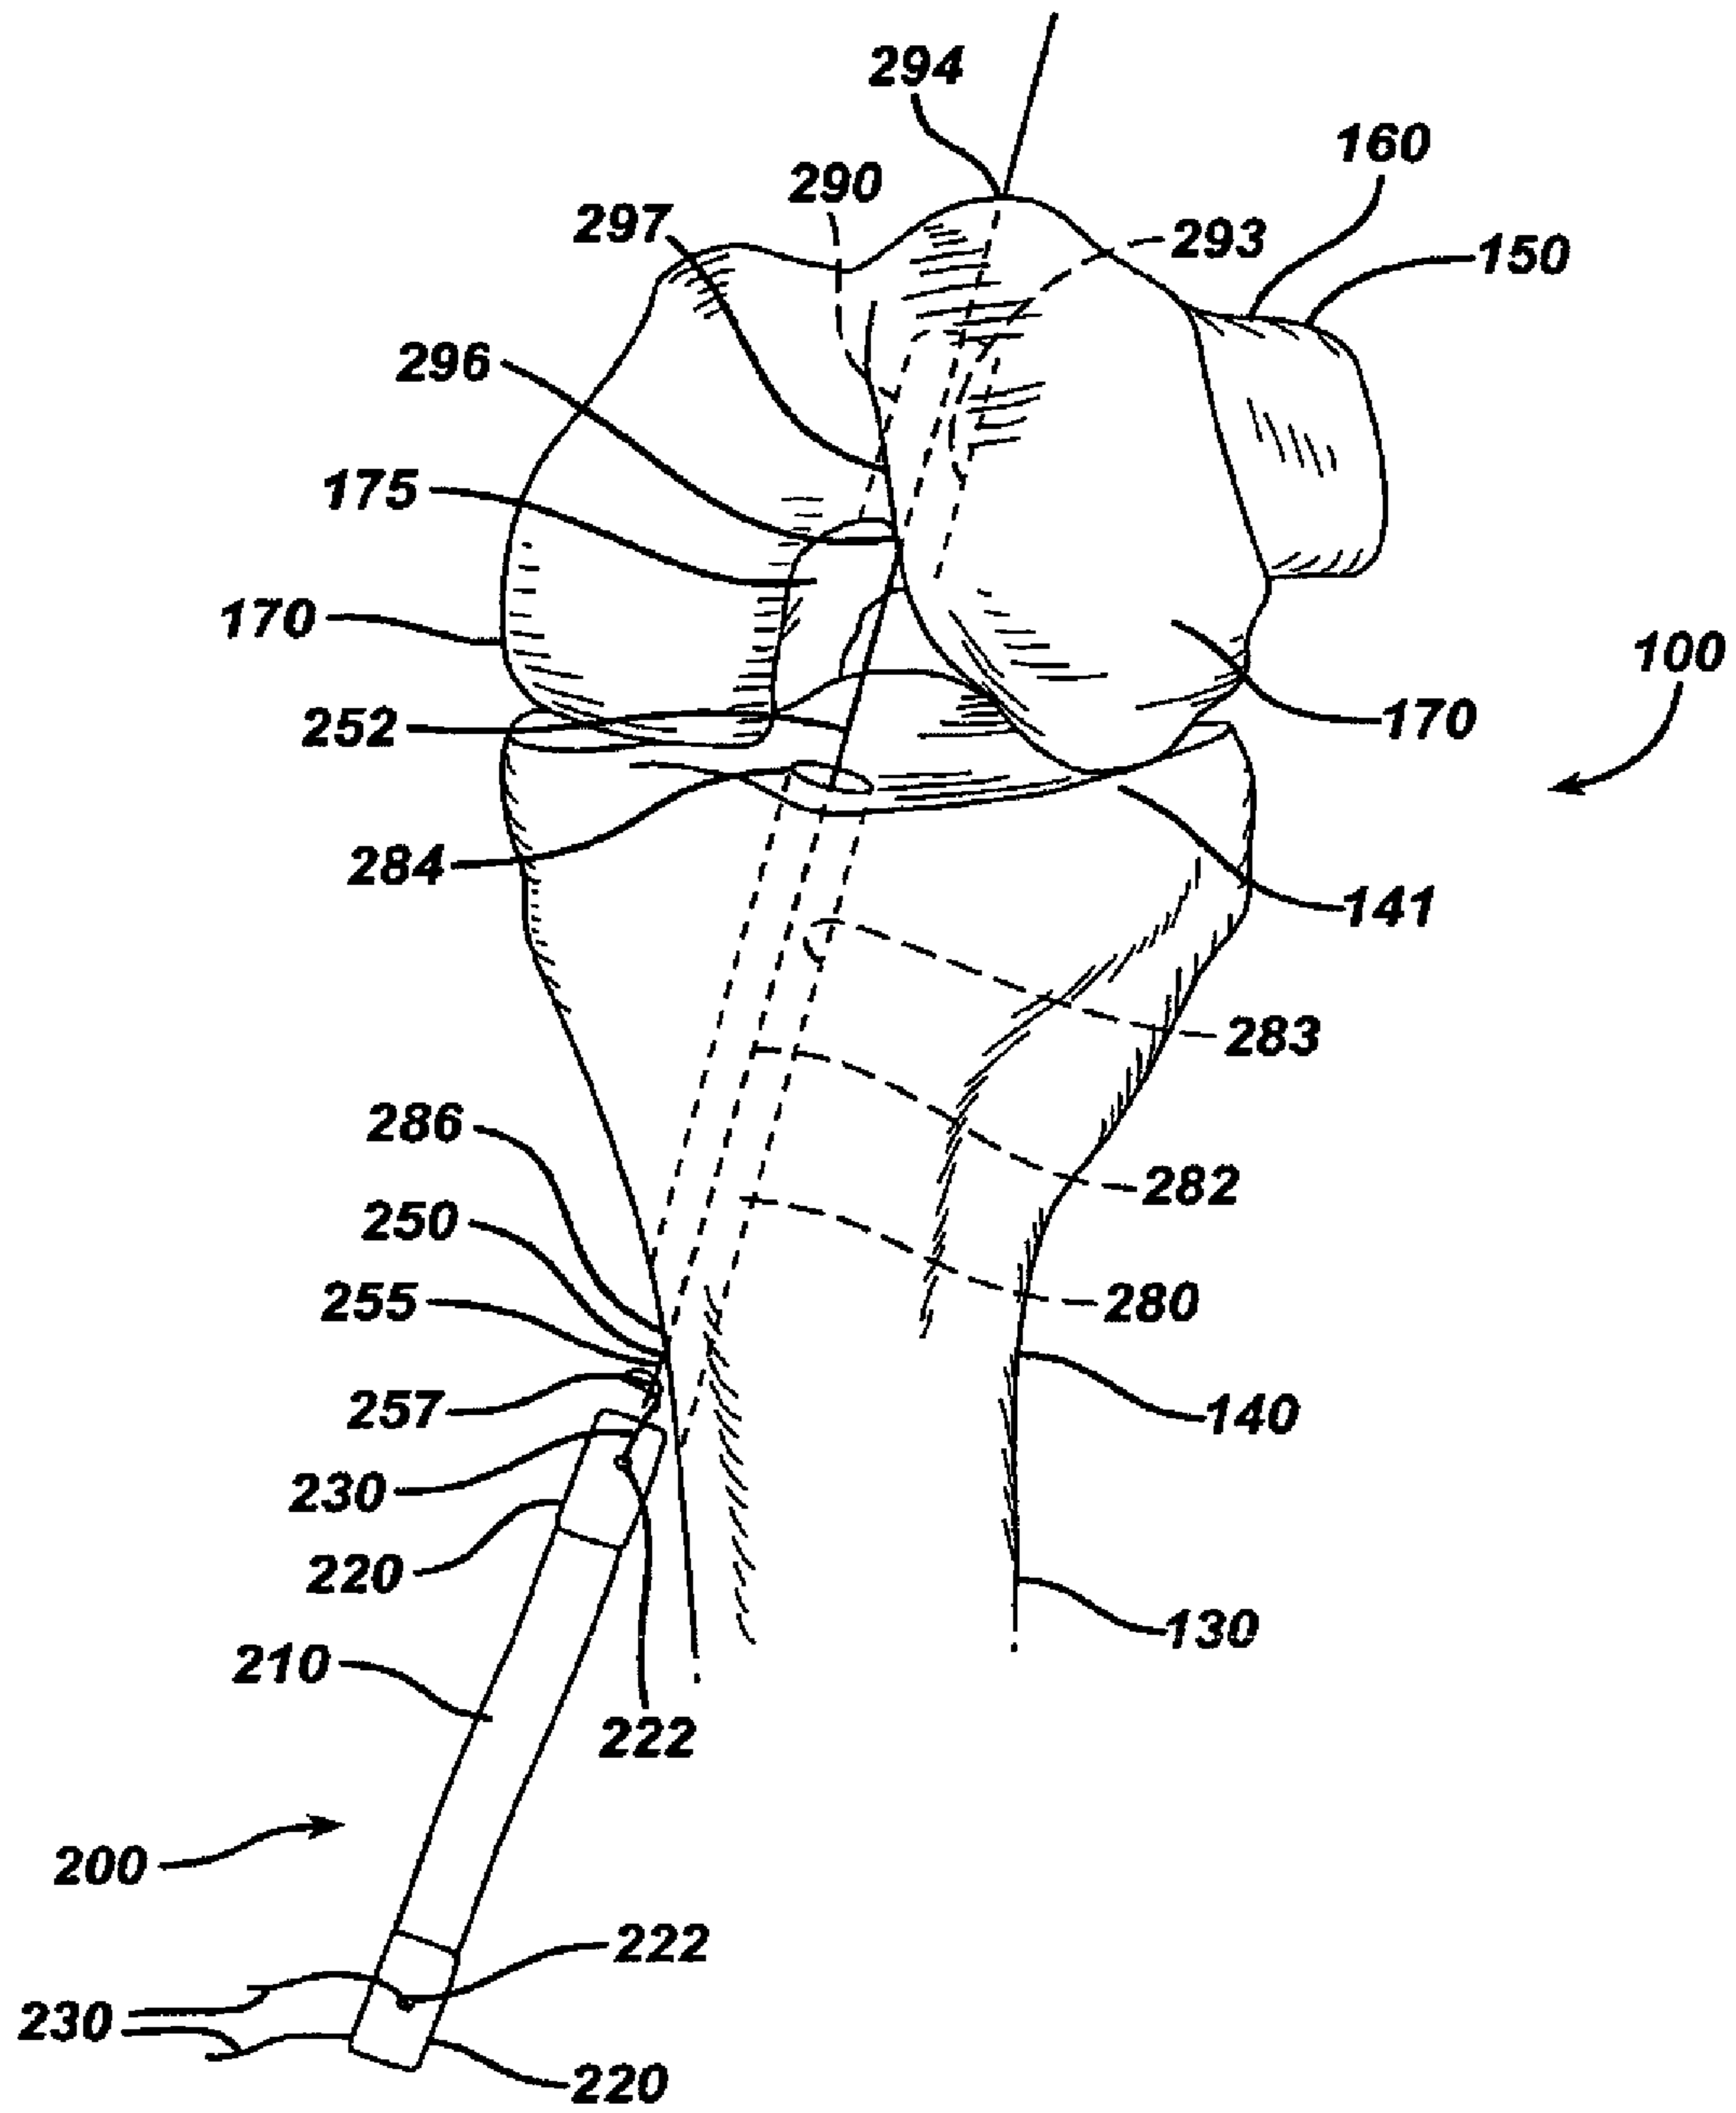


**FIG. 4**

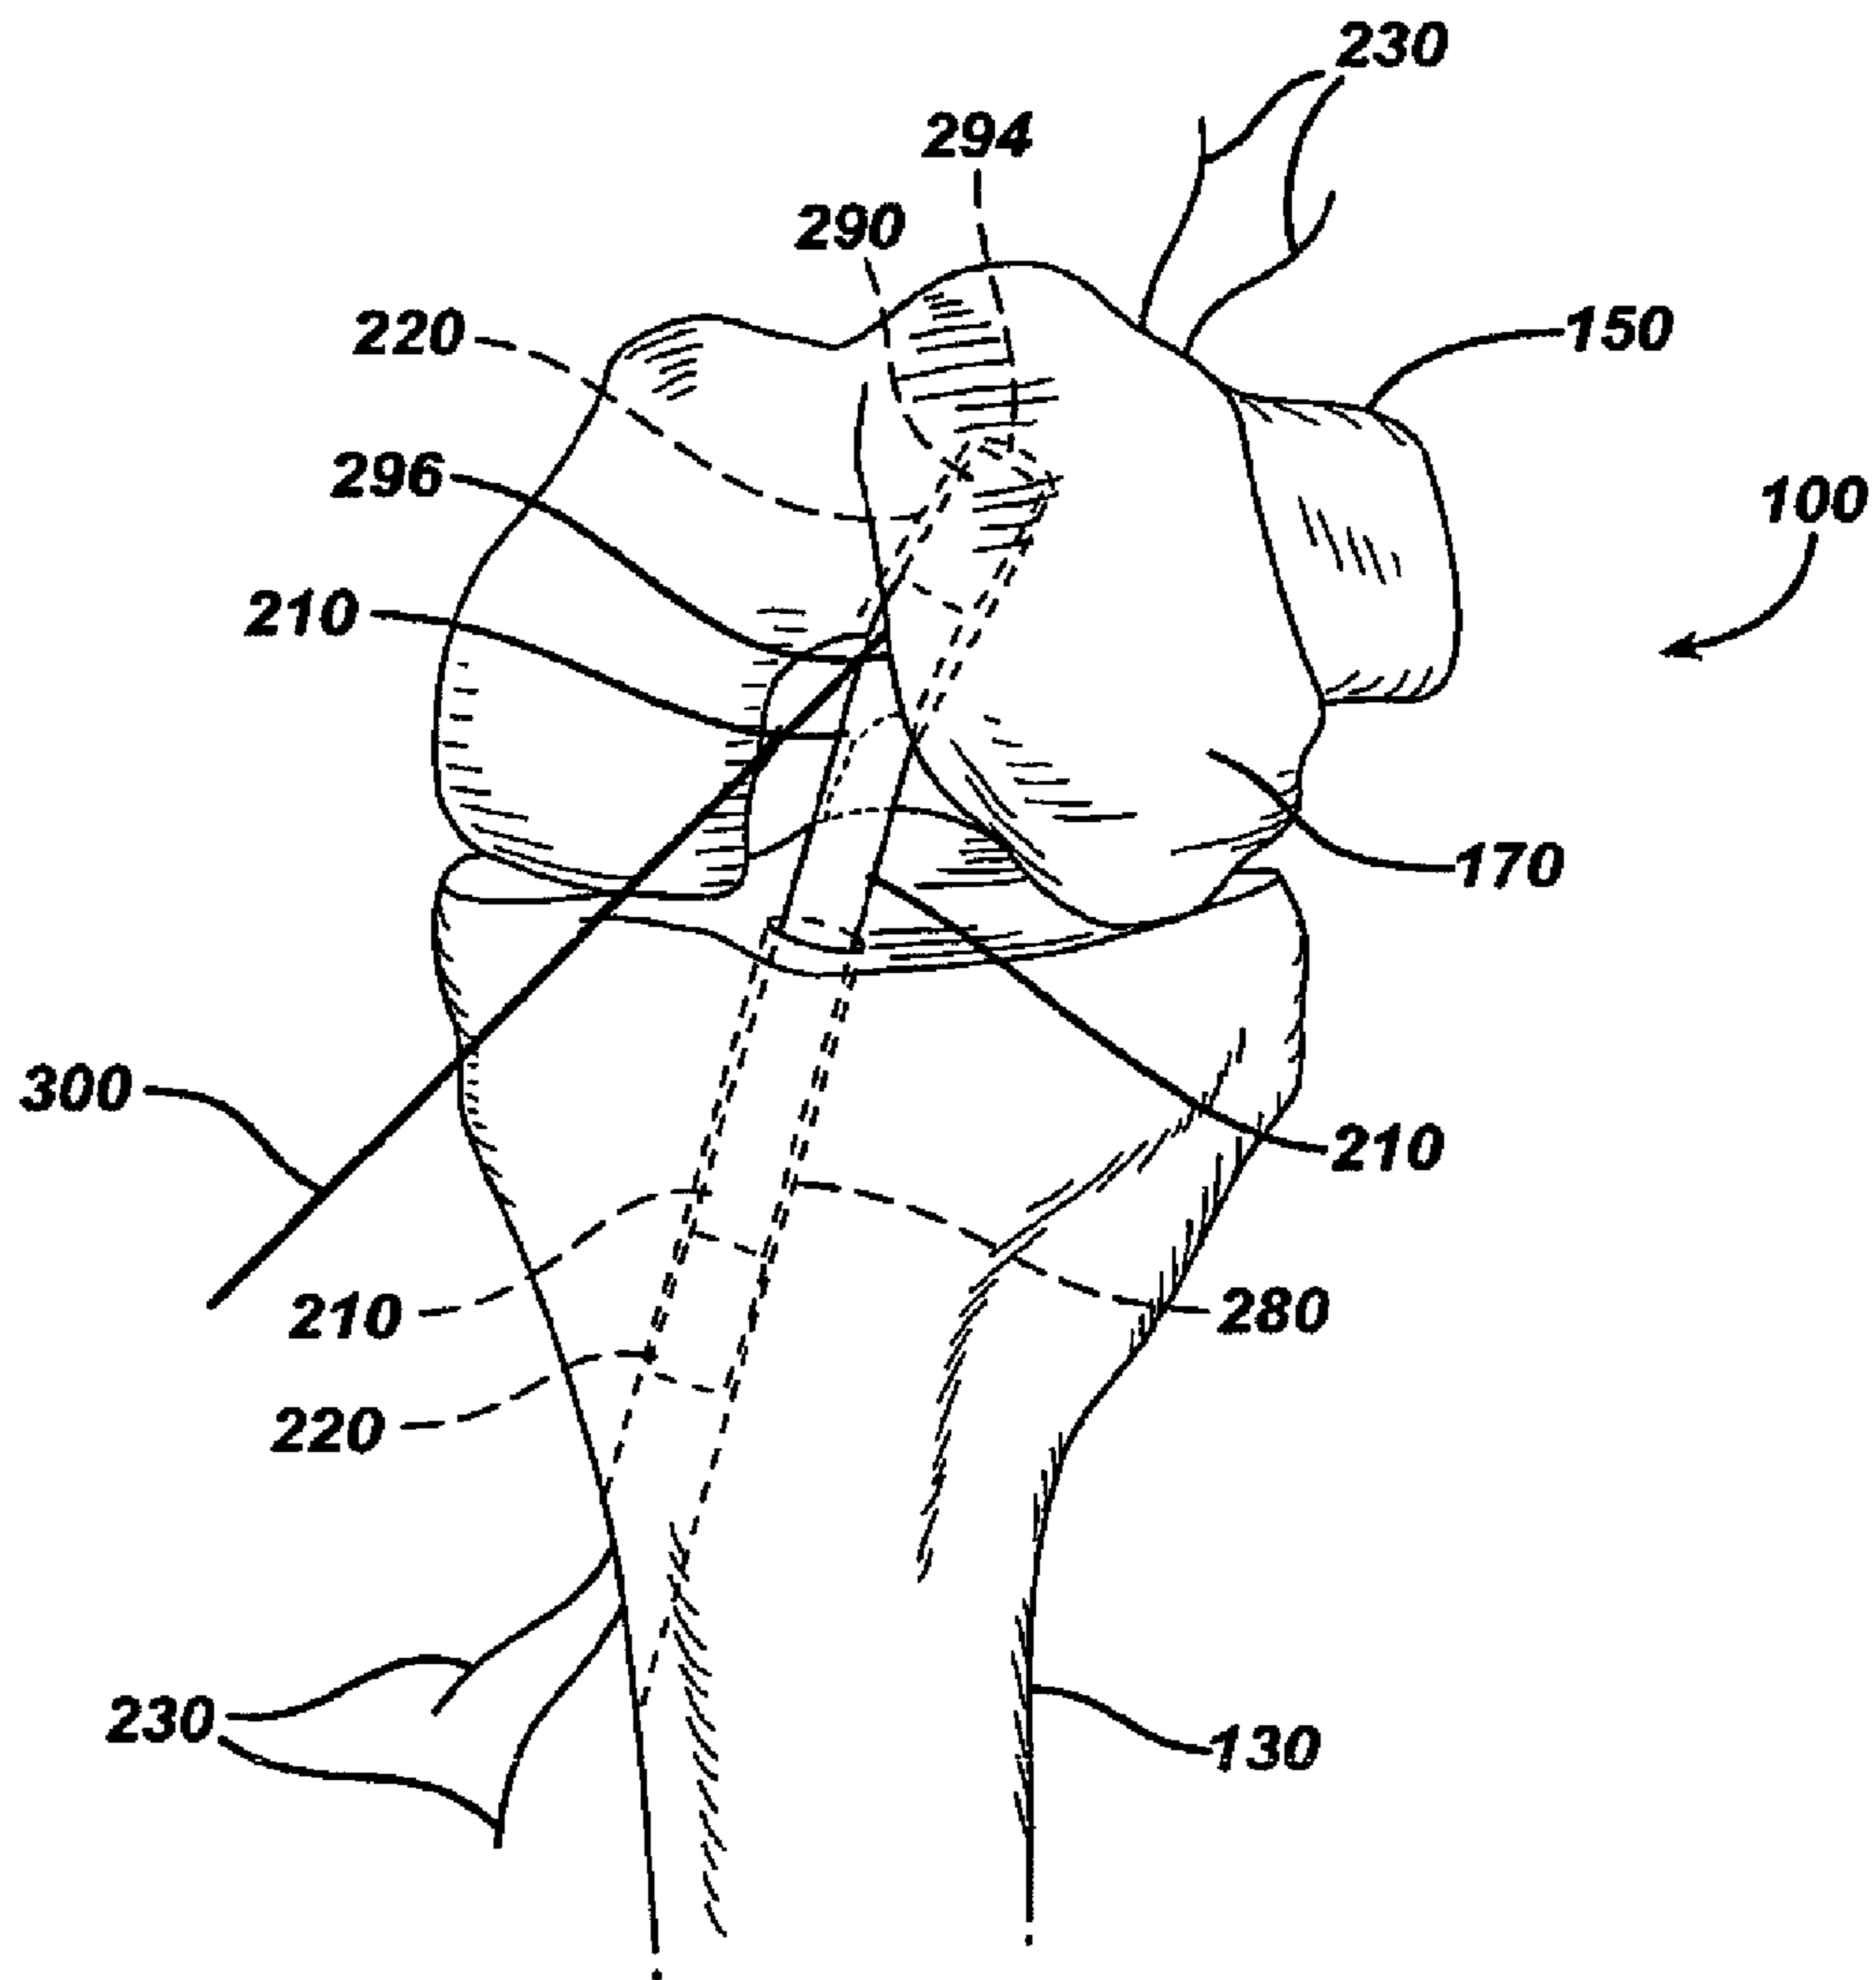

**FIG. 5**

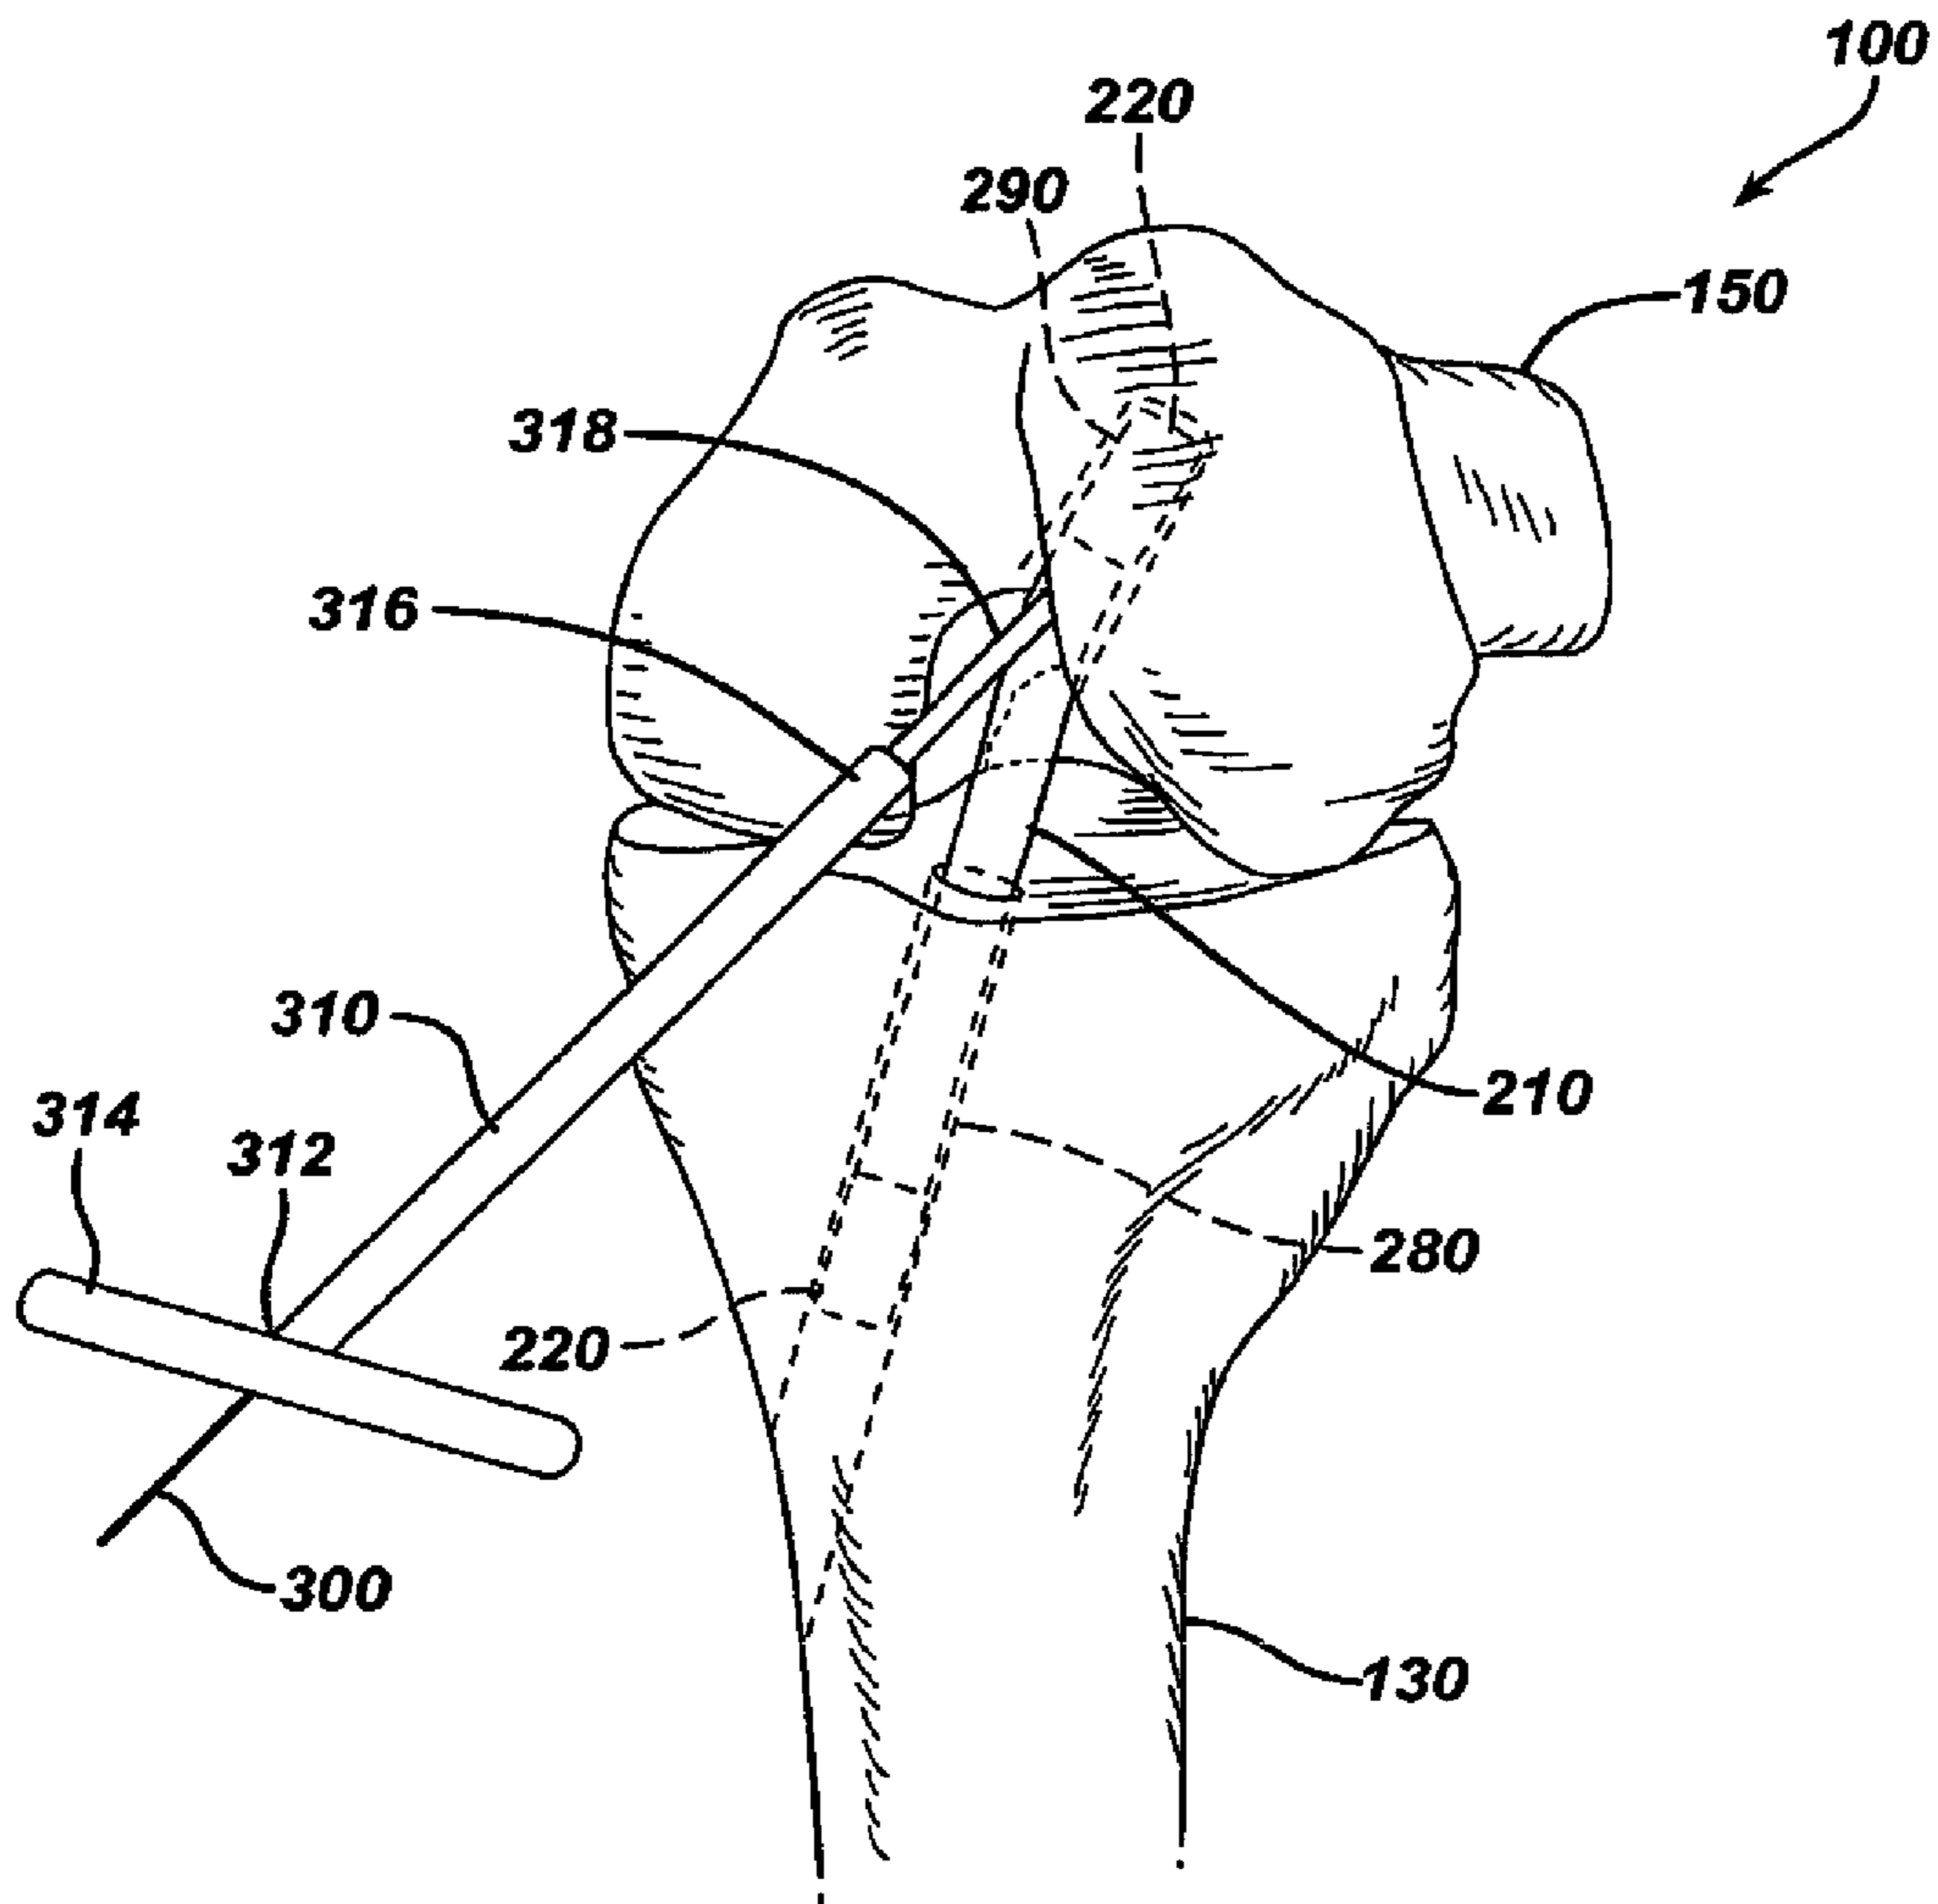



**FIG. 6**

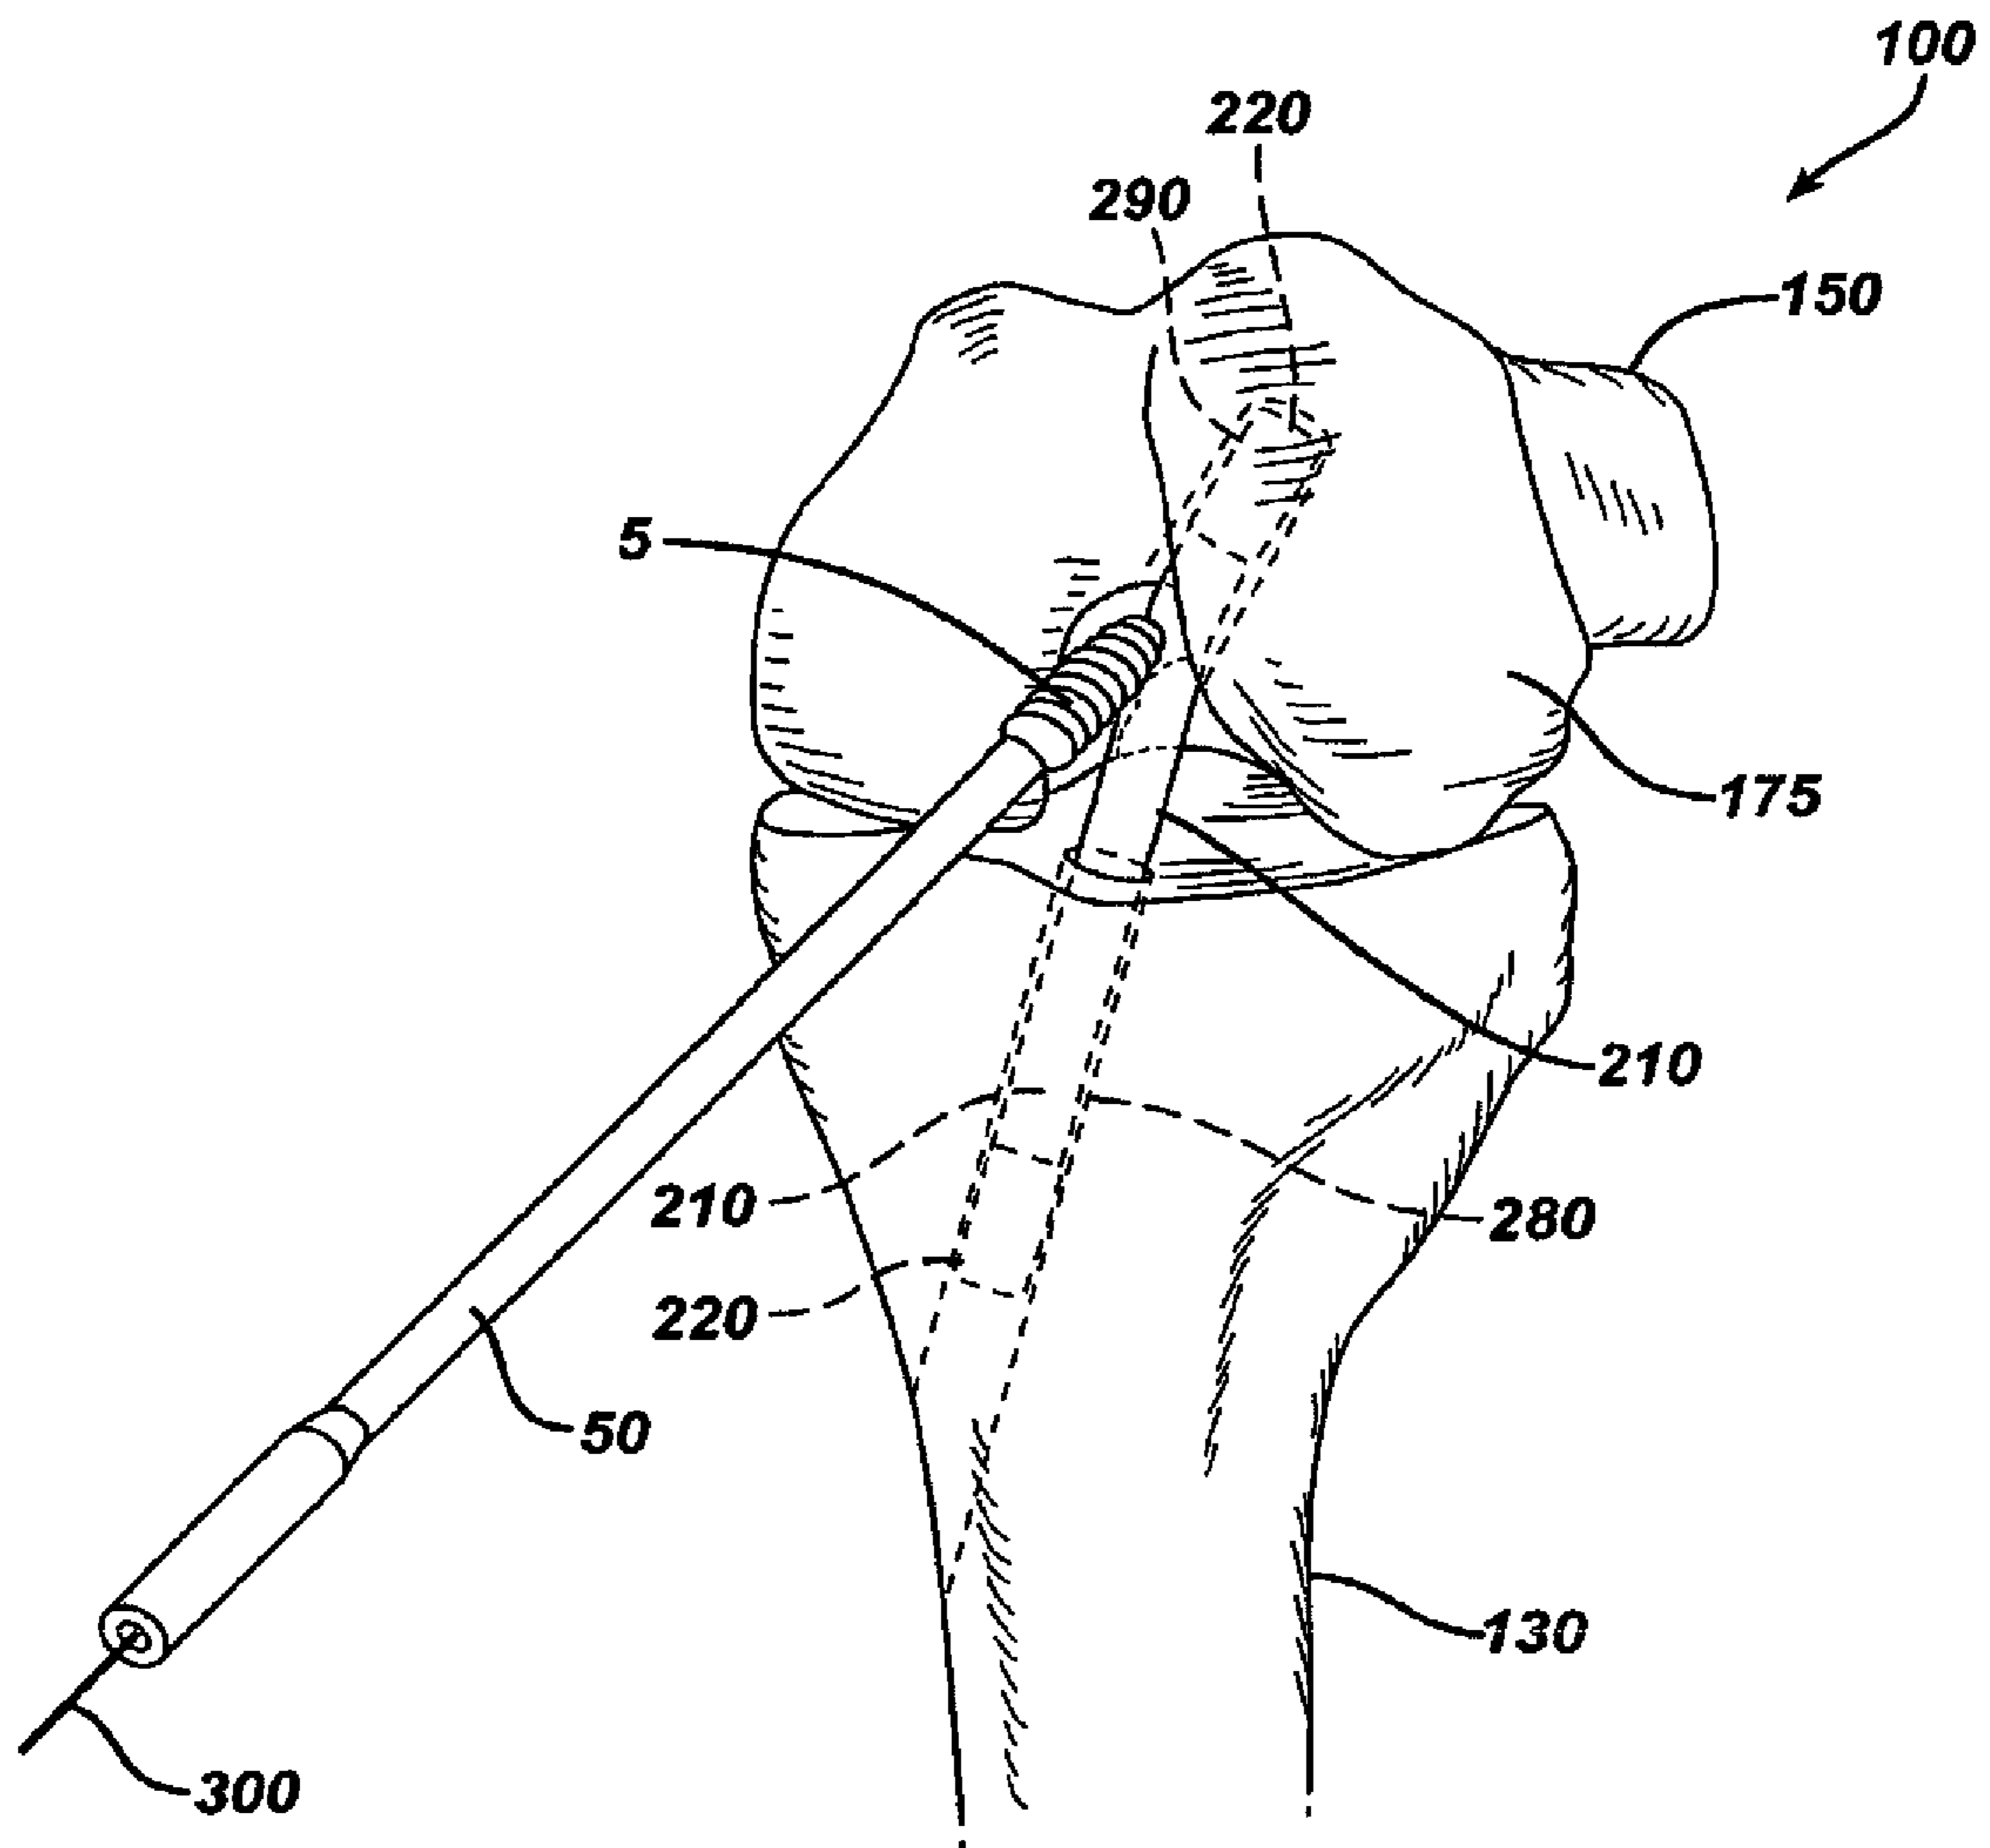





**FIG. 7**

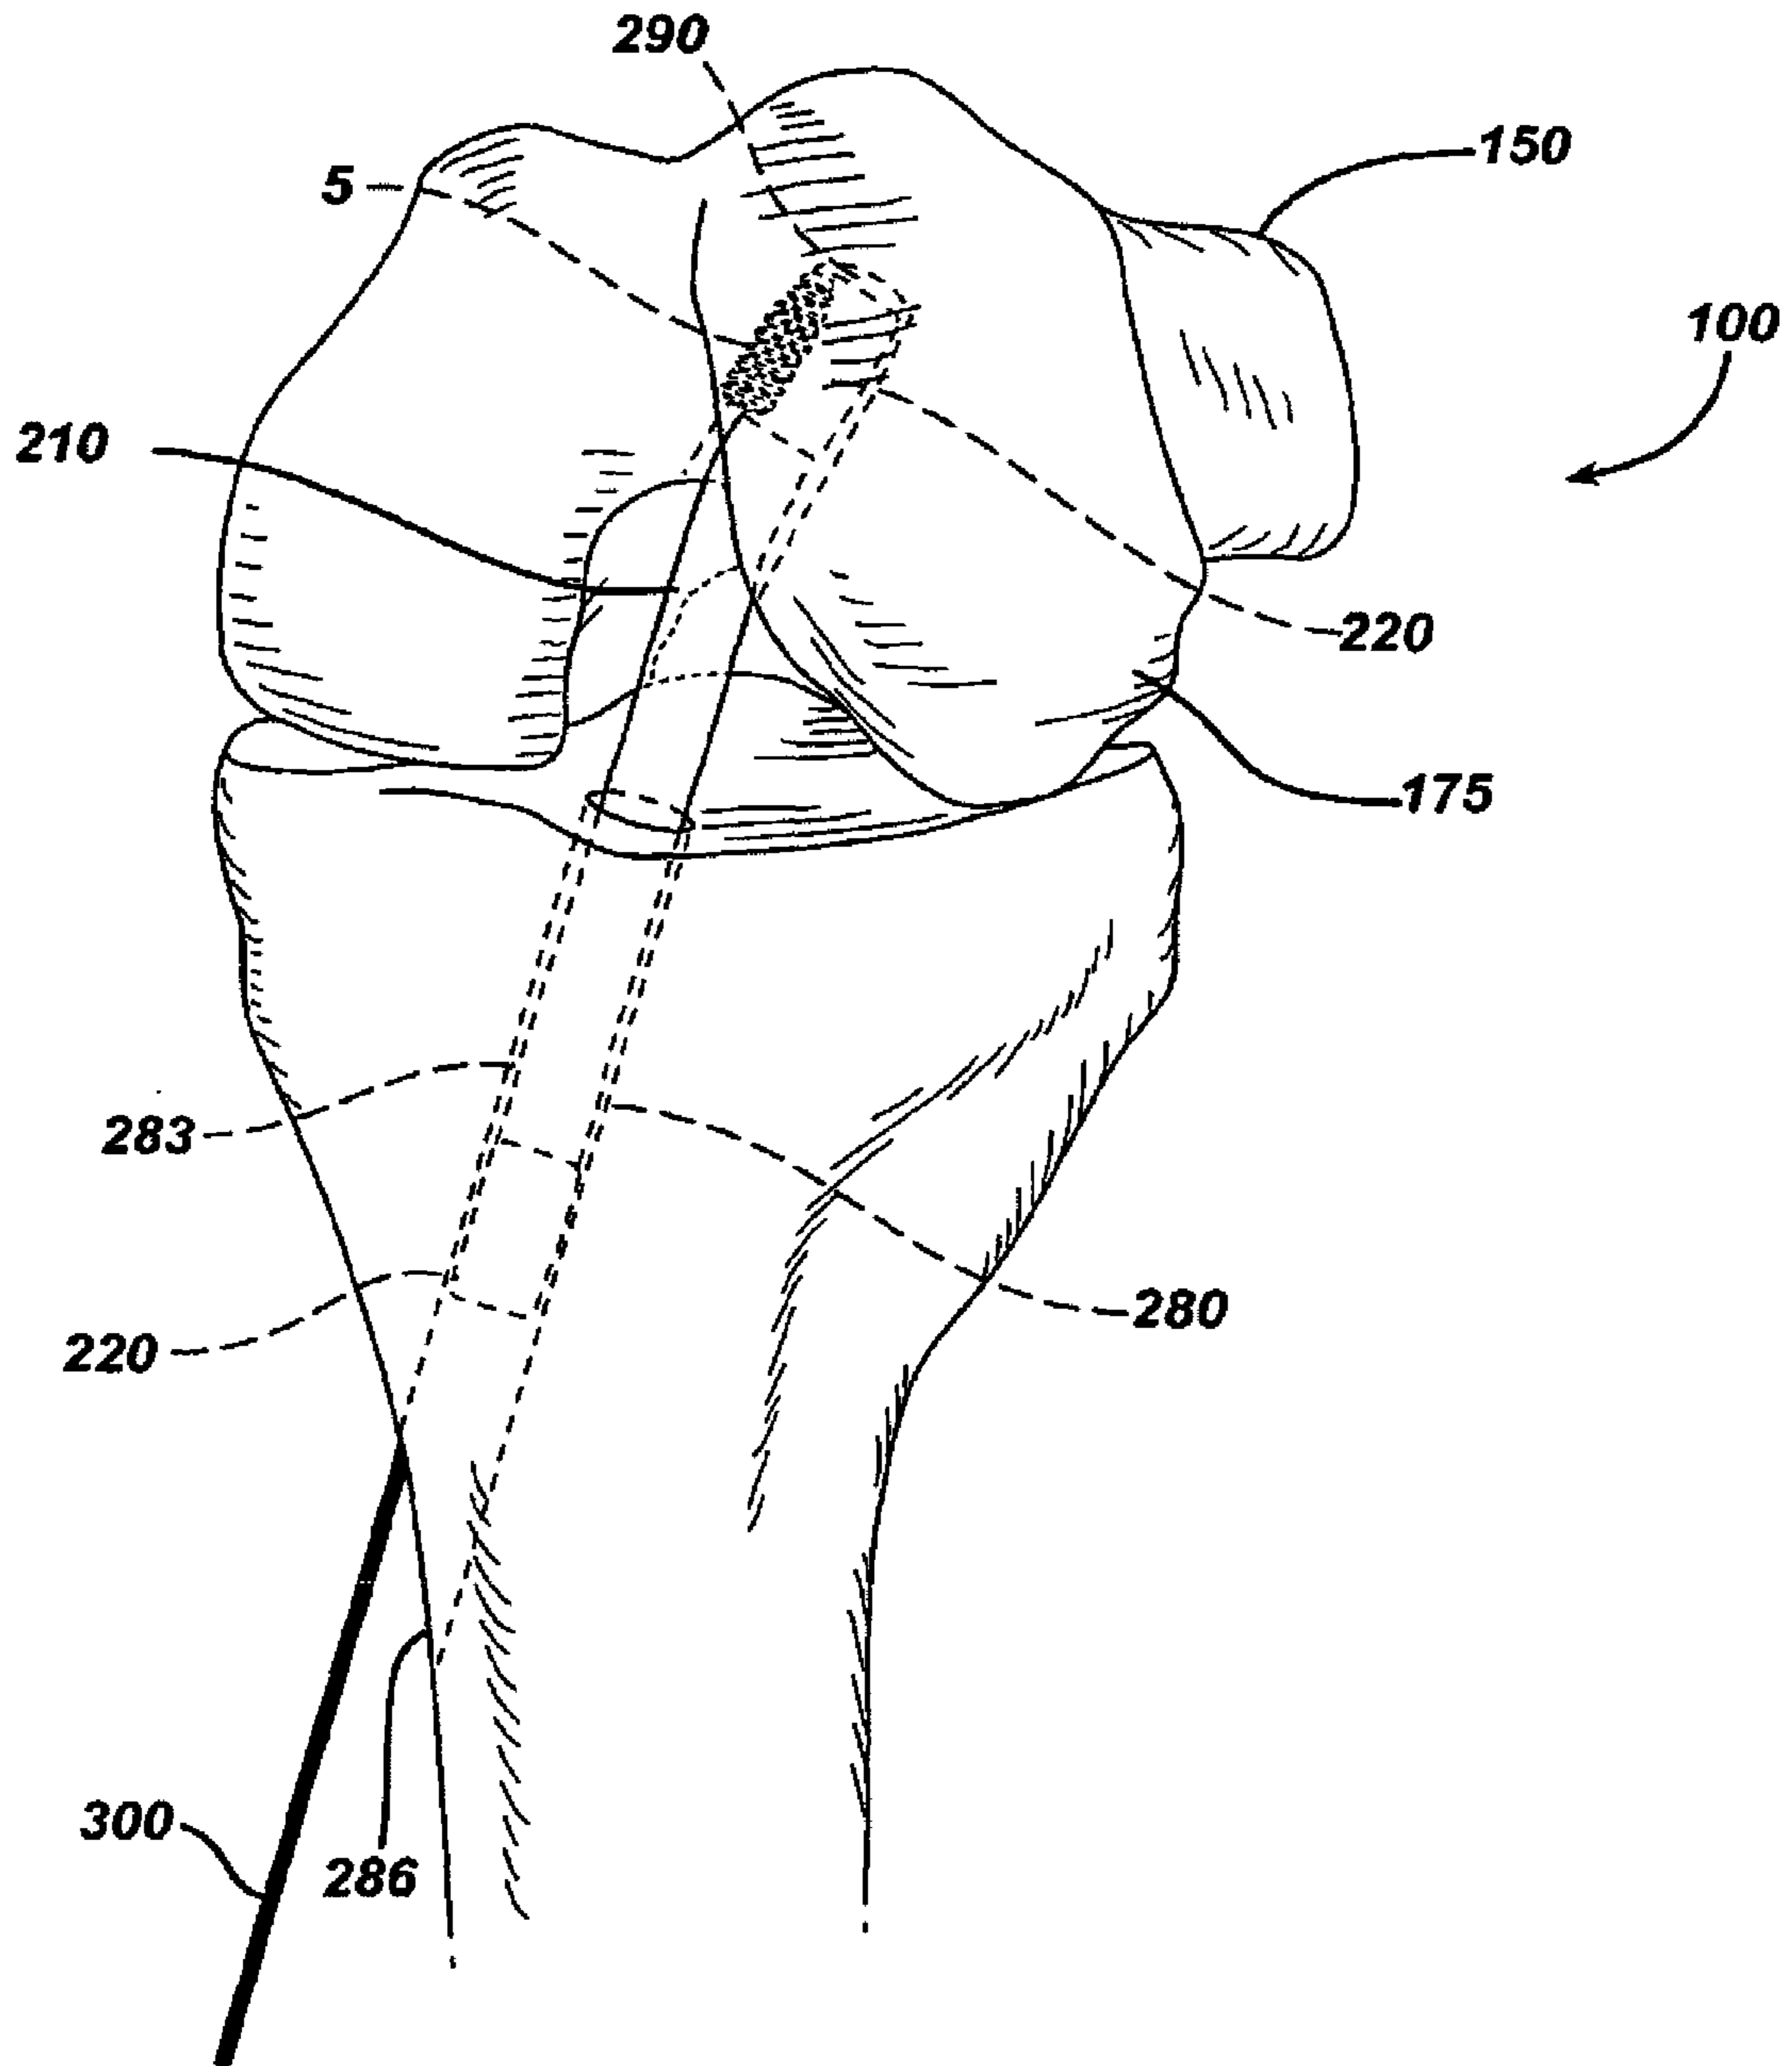

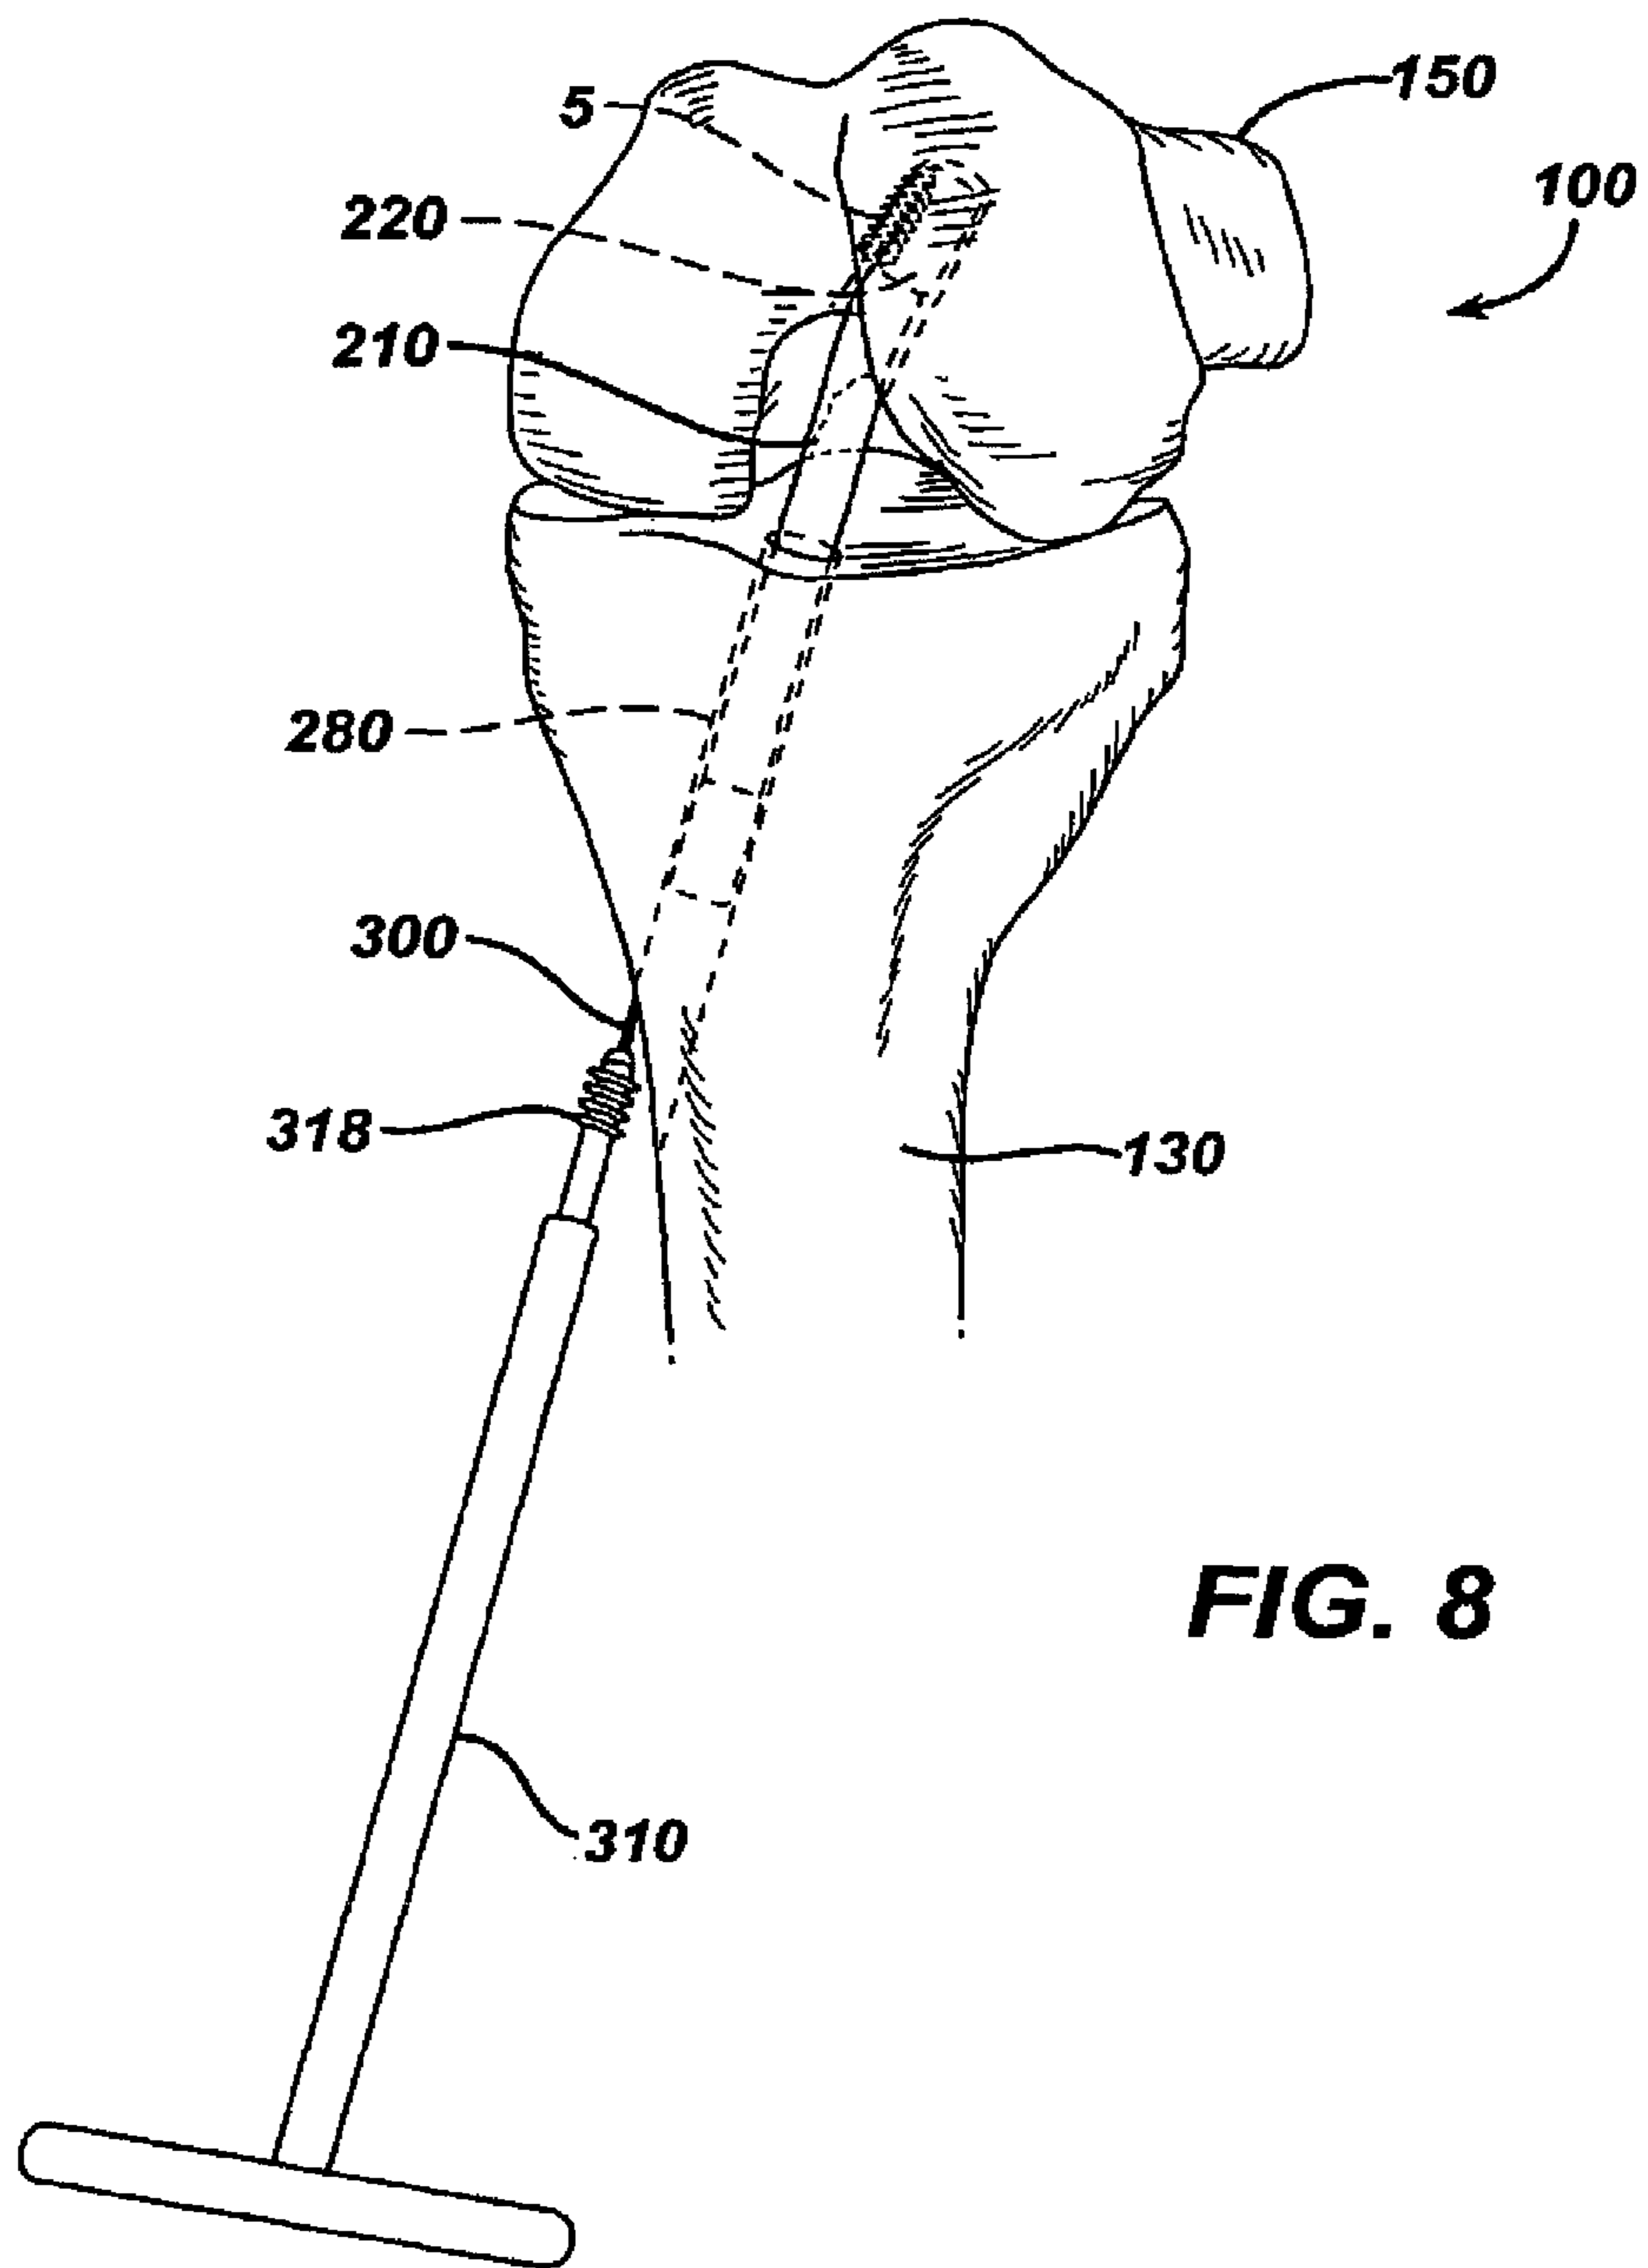


**FIG. 8**

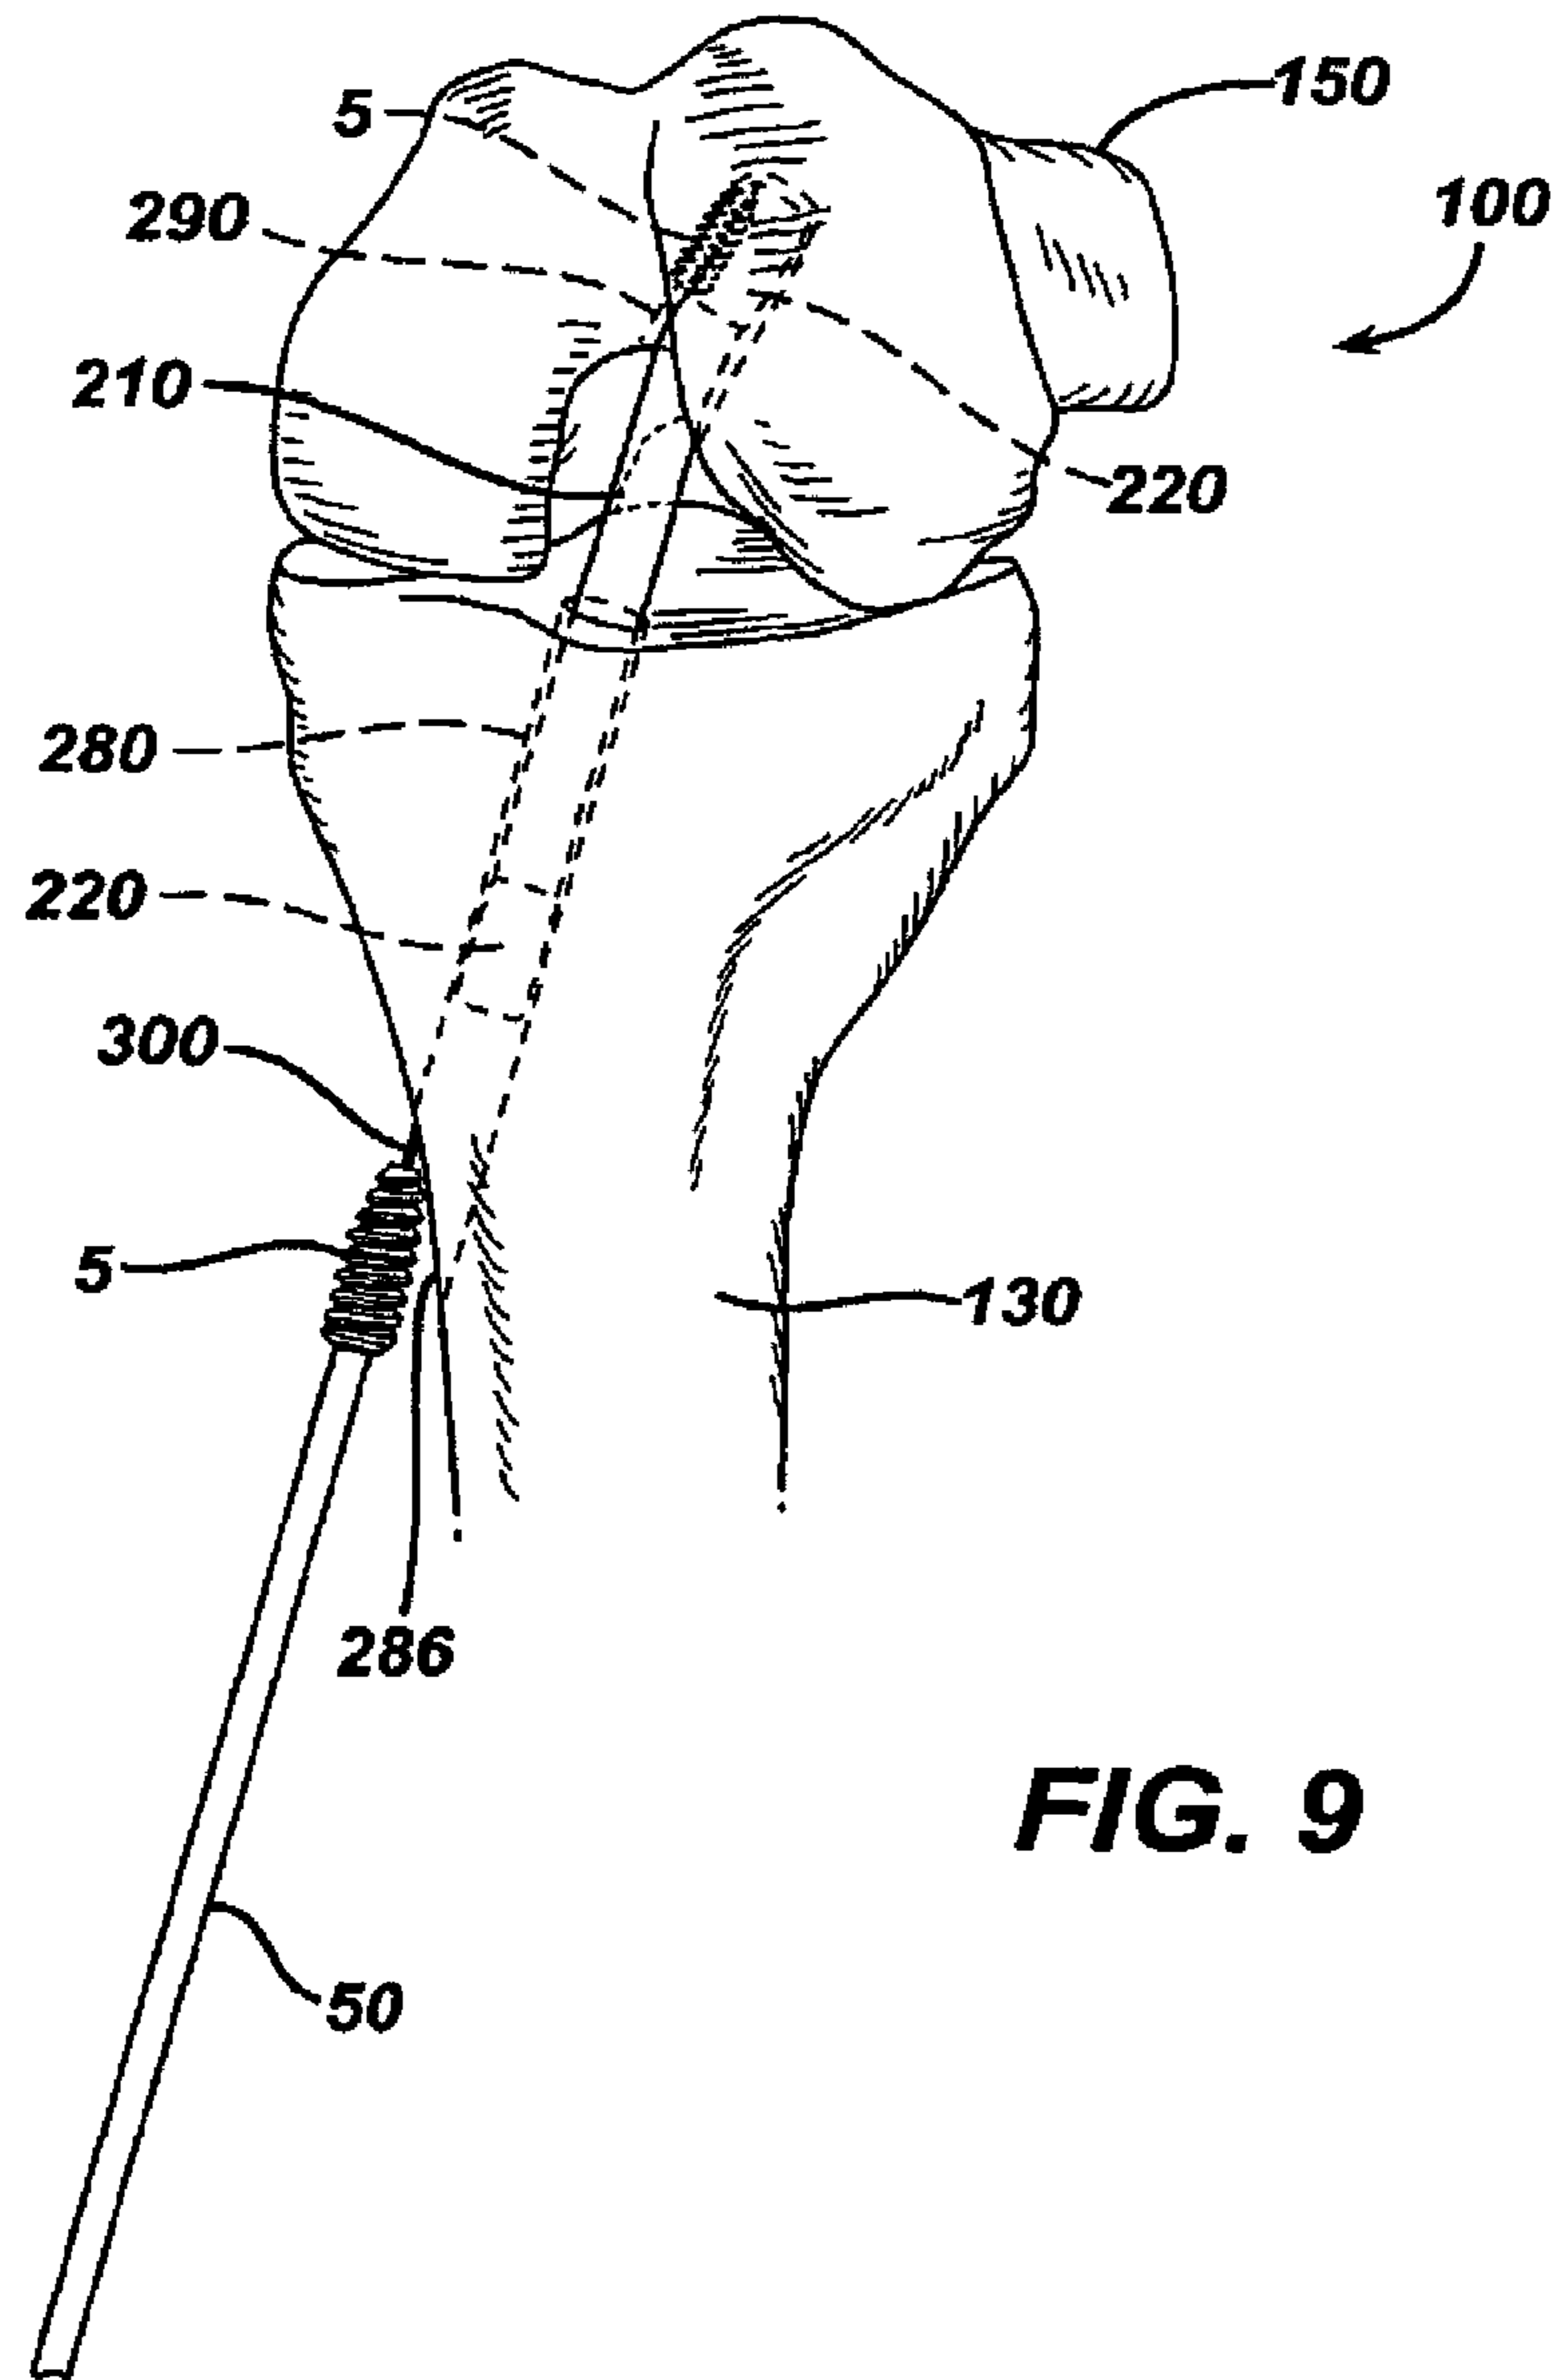

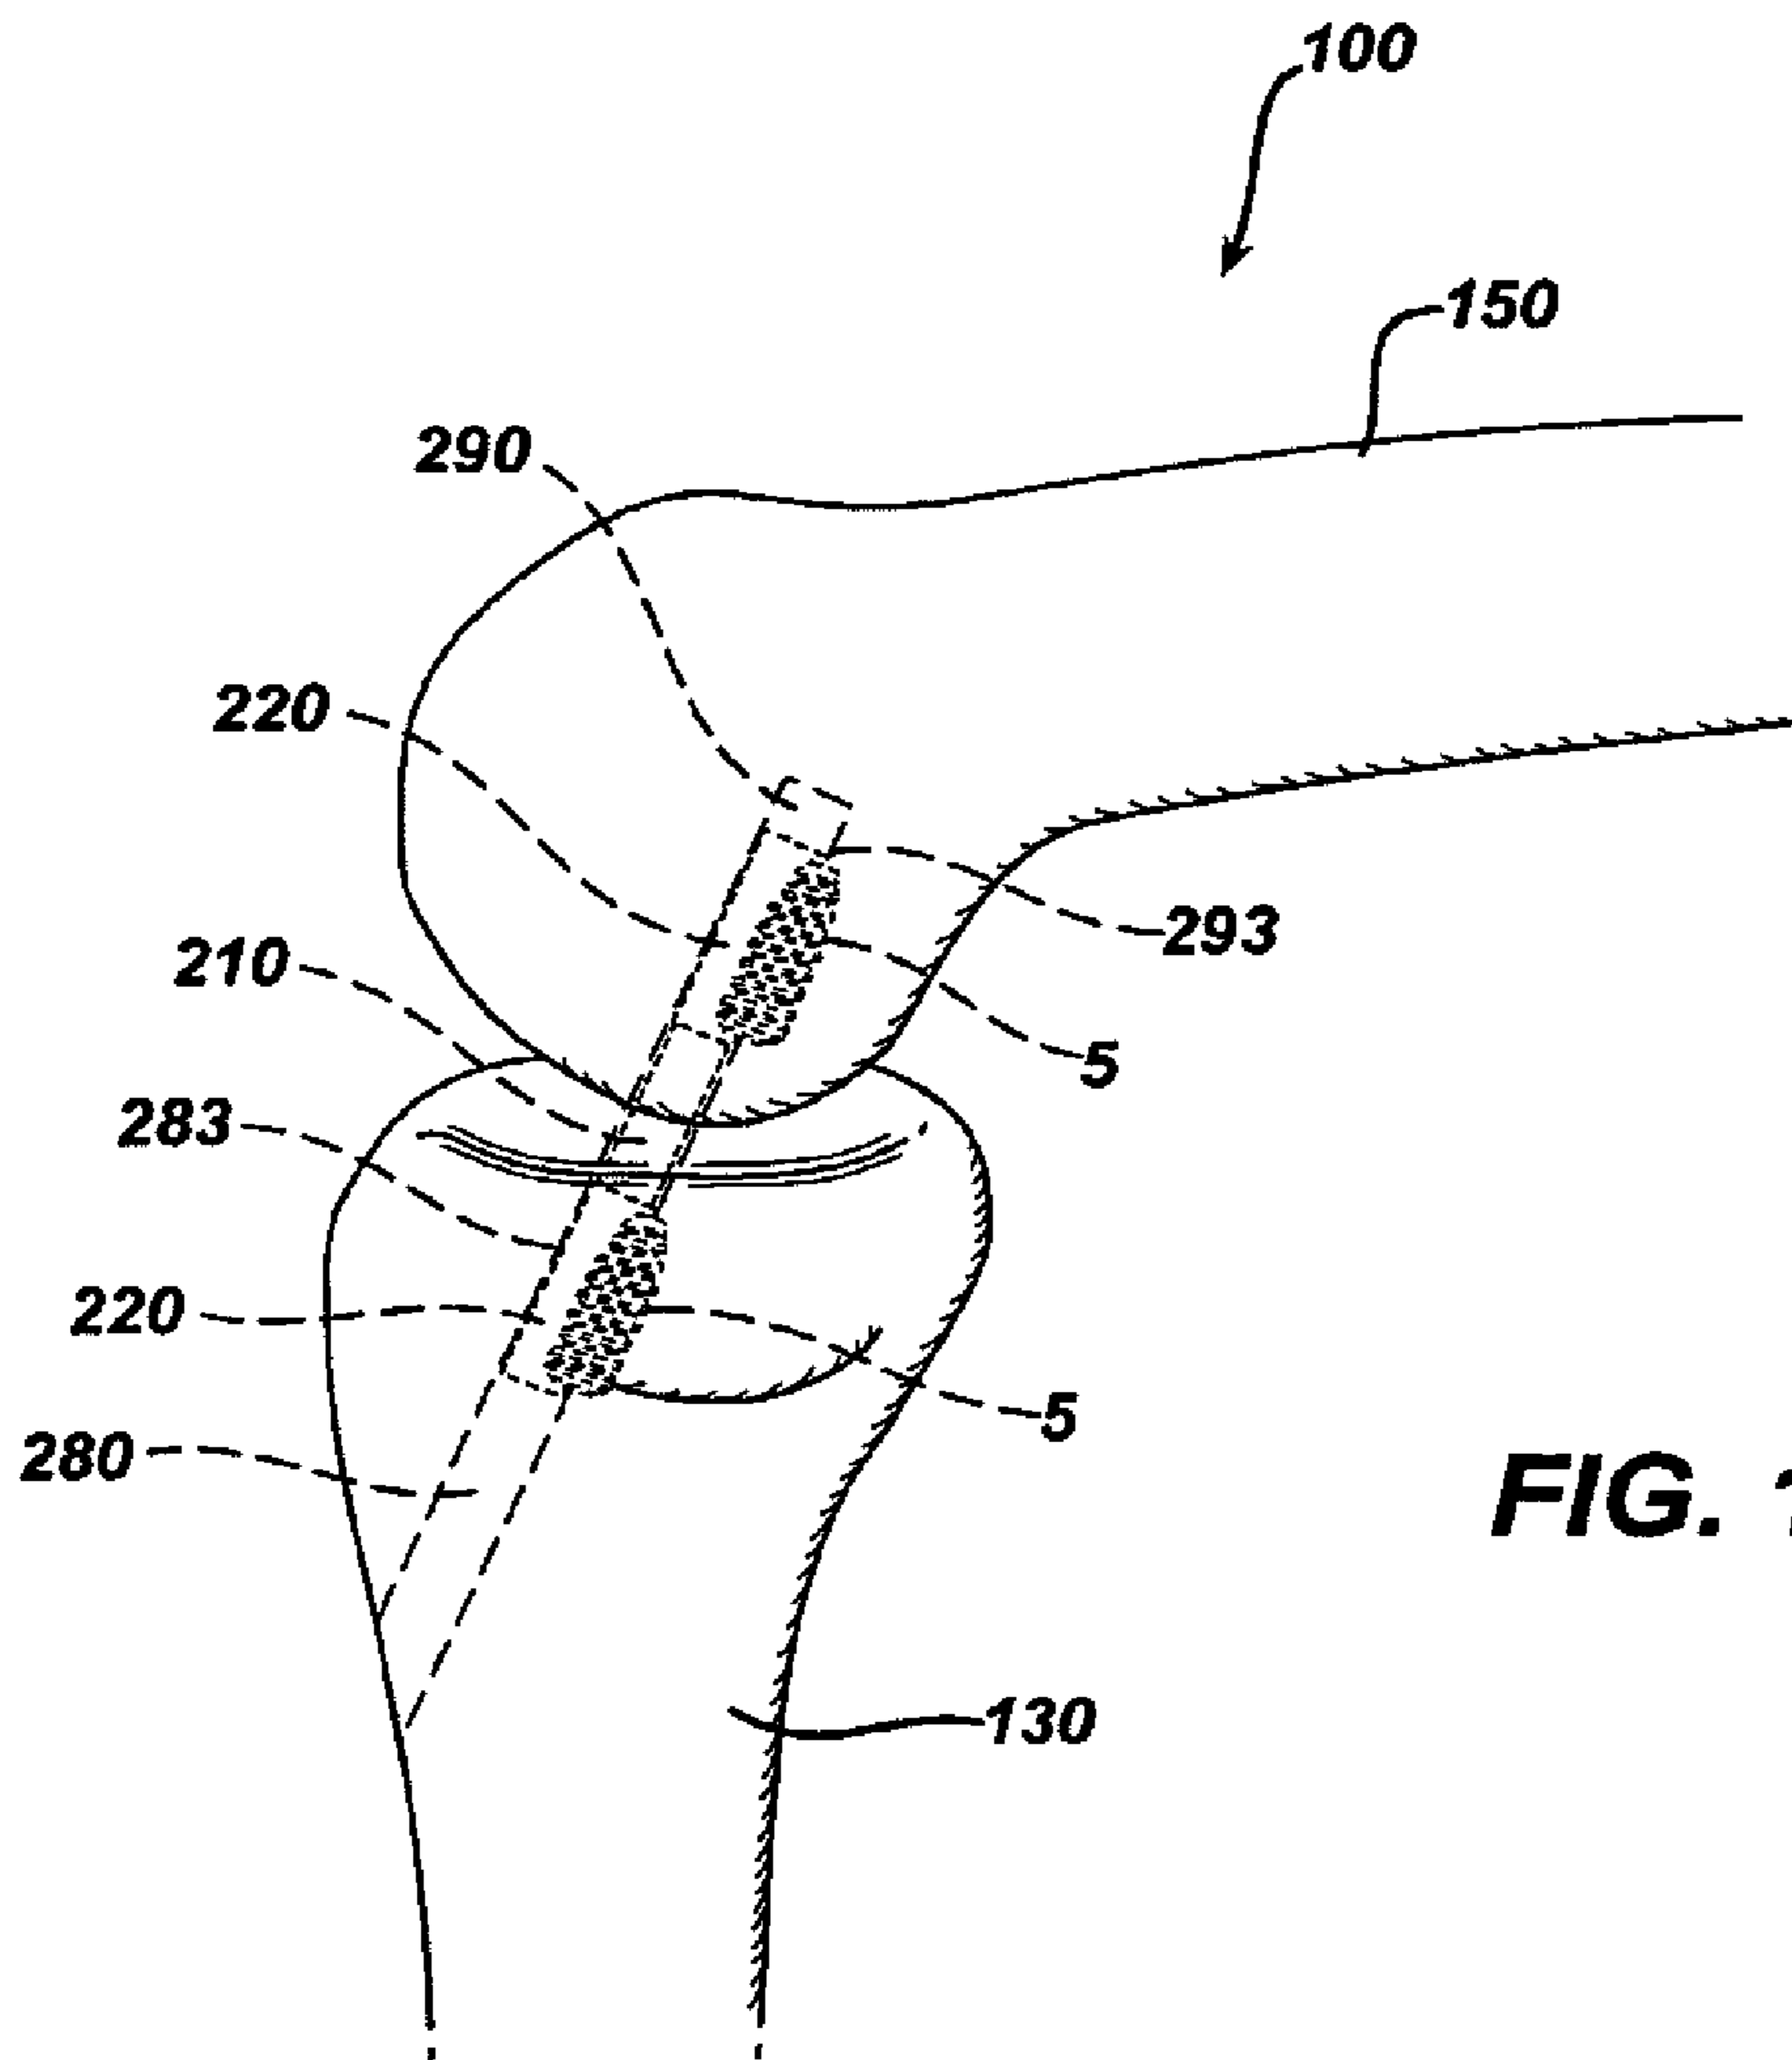

**FIG. 10**


**FIG. 11A**

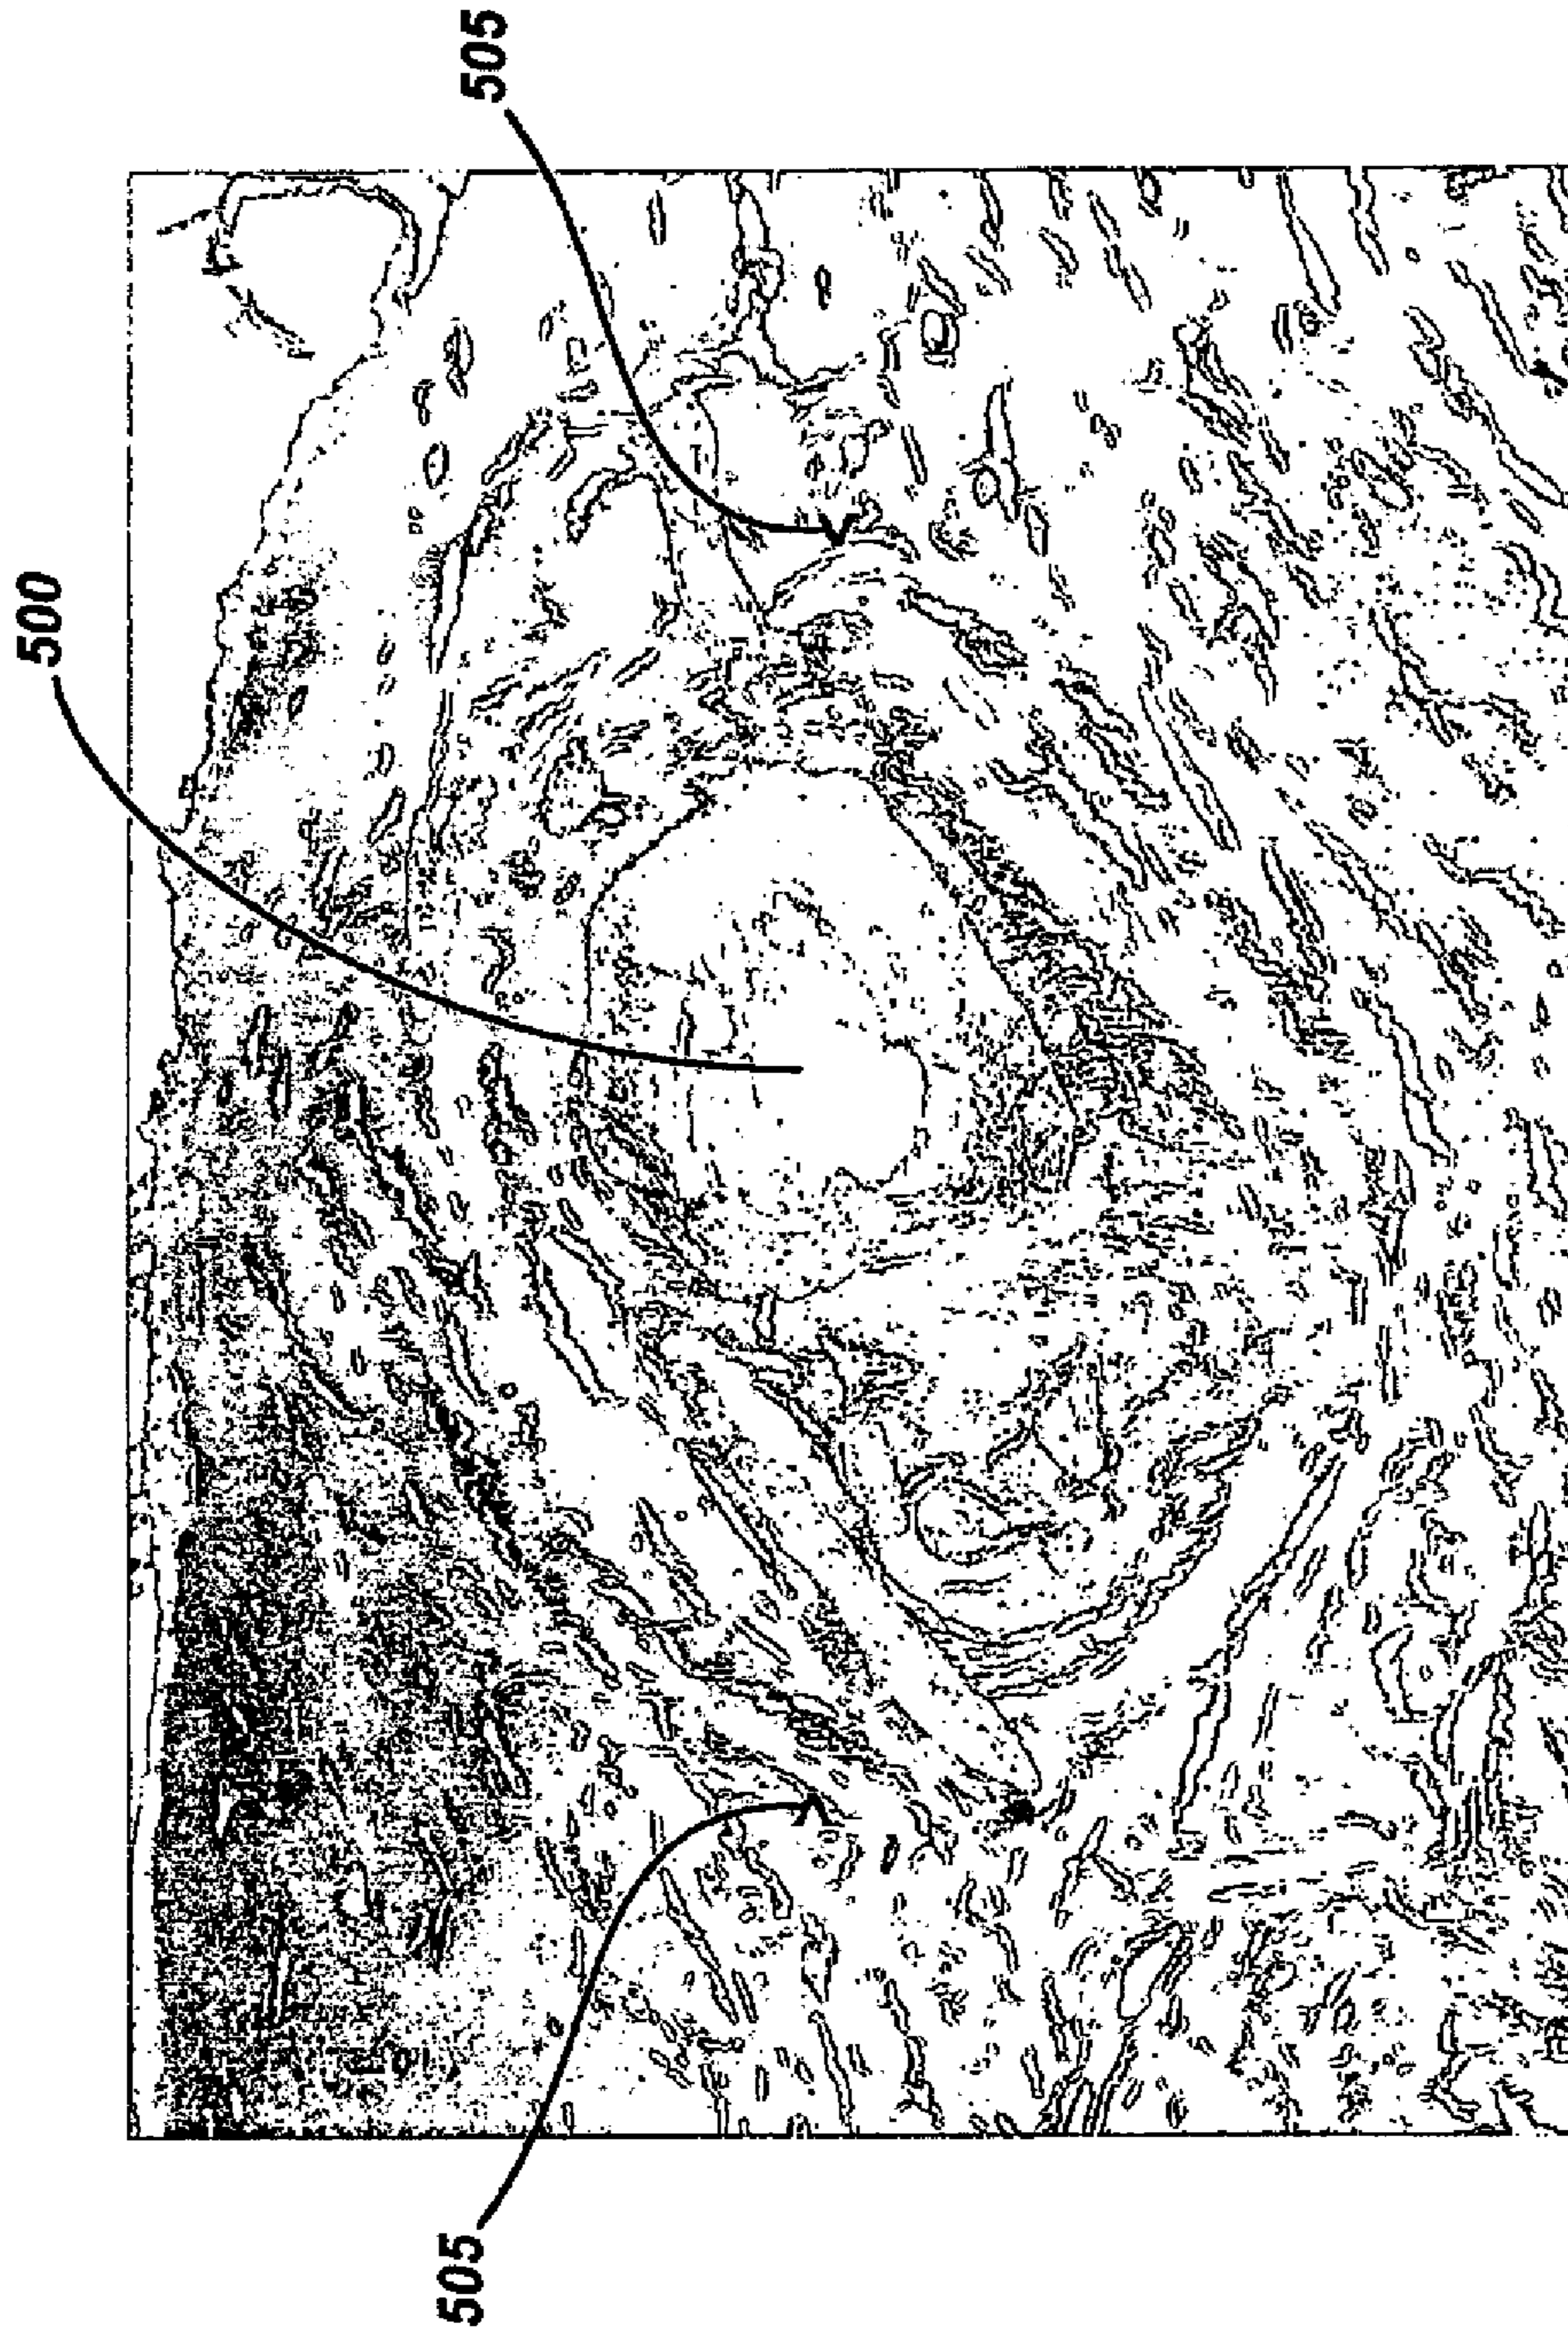

Distance between arrows ~3.5mm




**FIG. 11B**

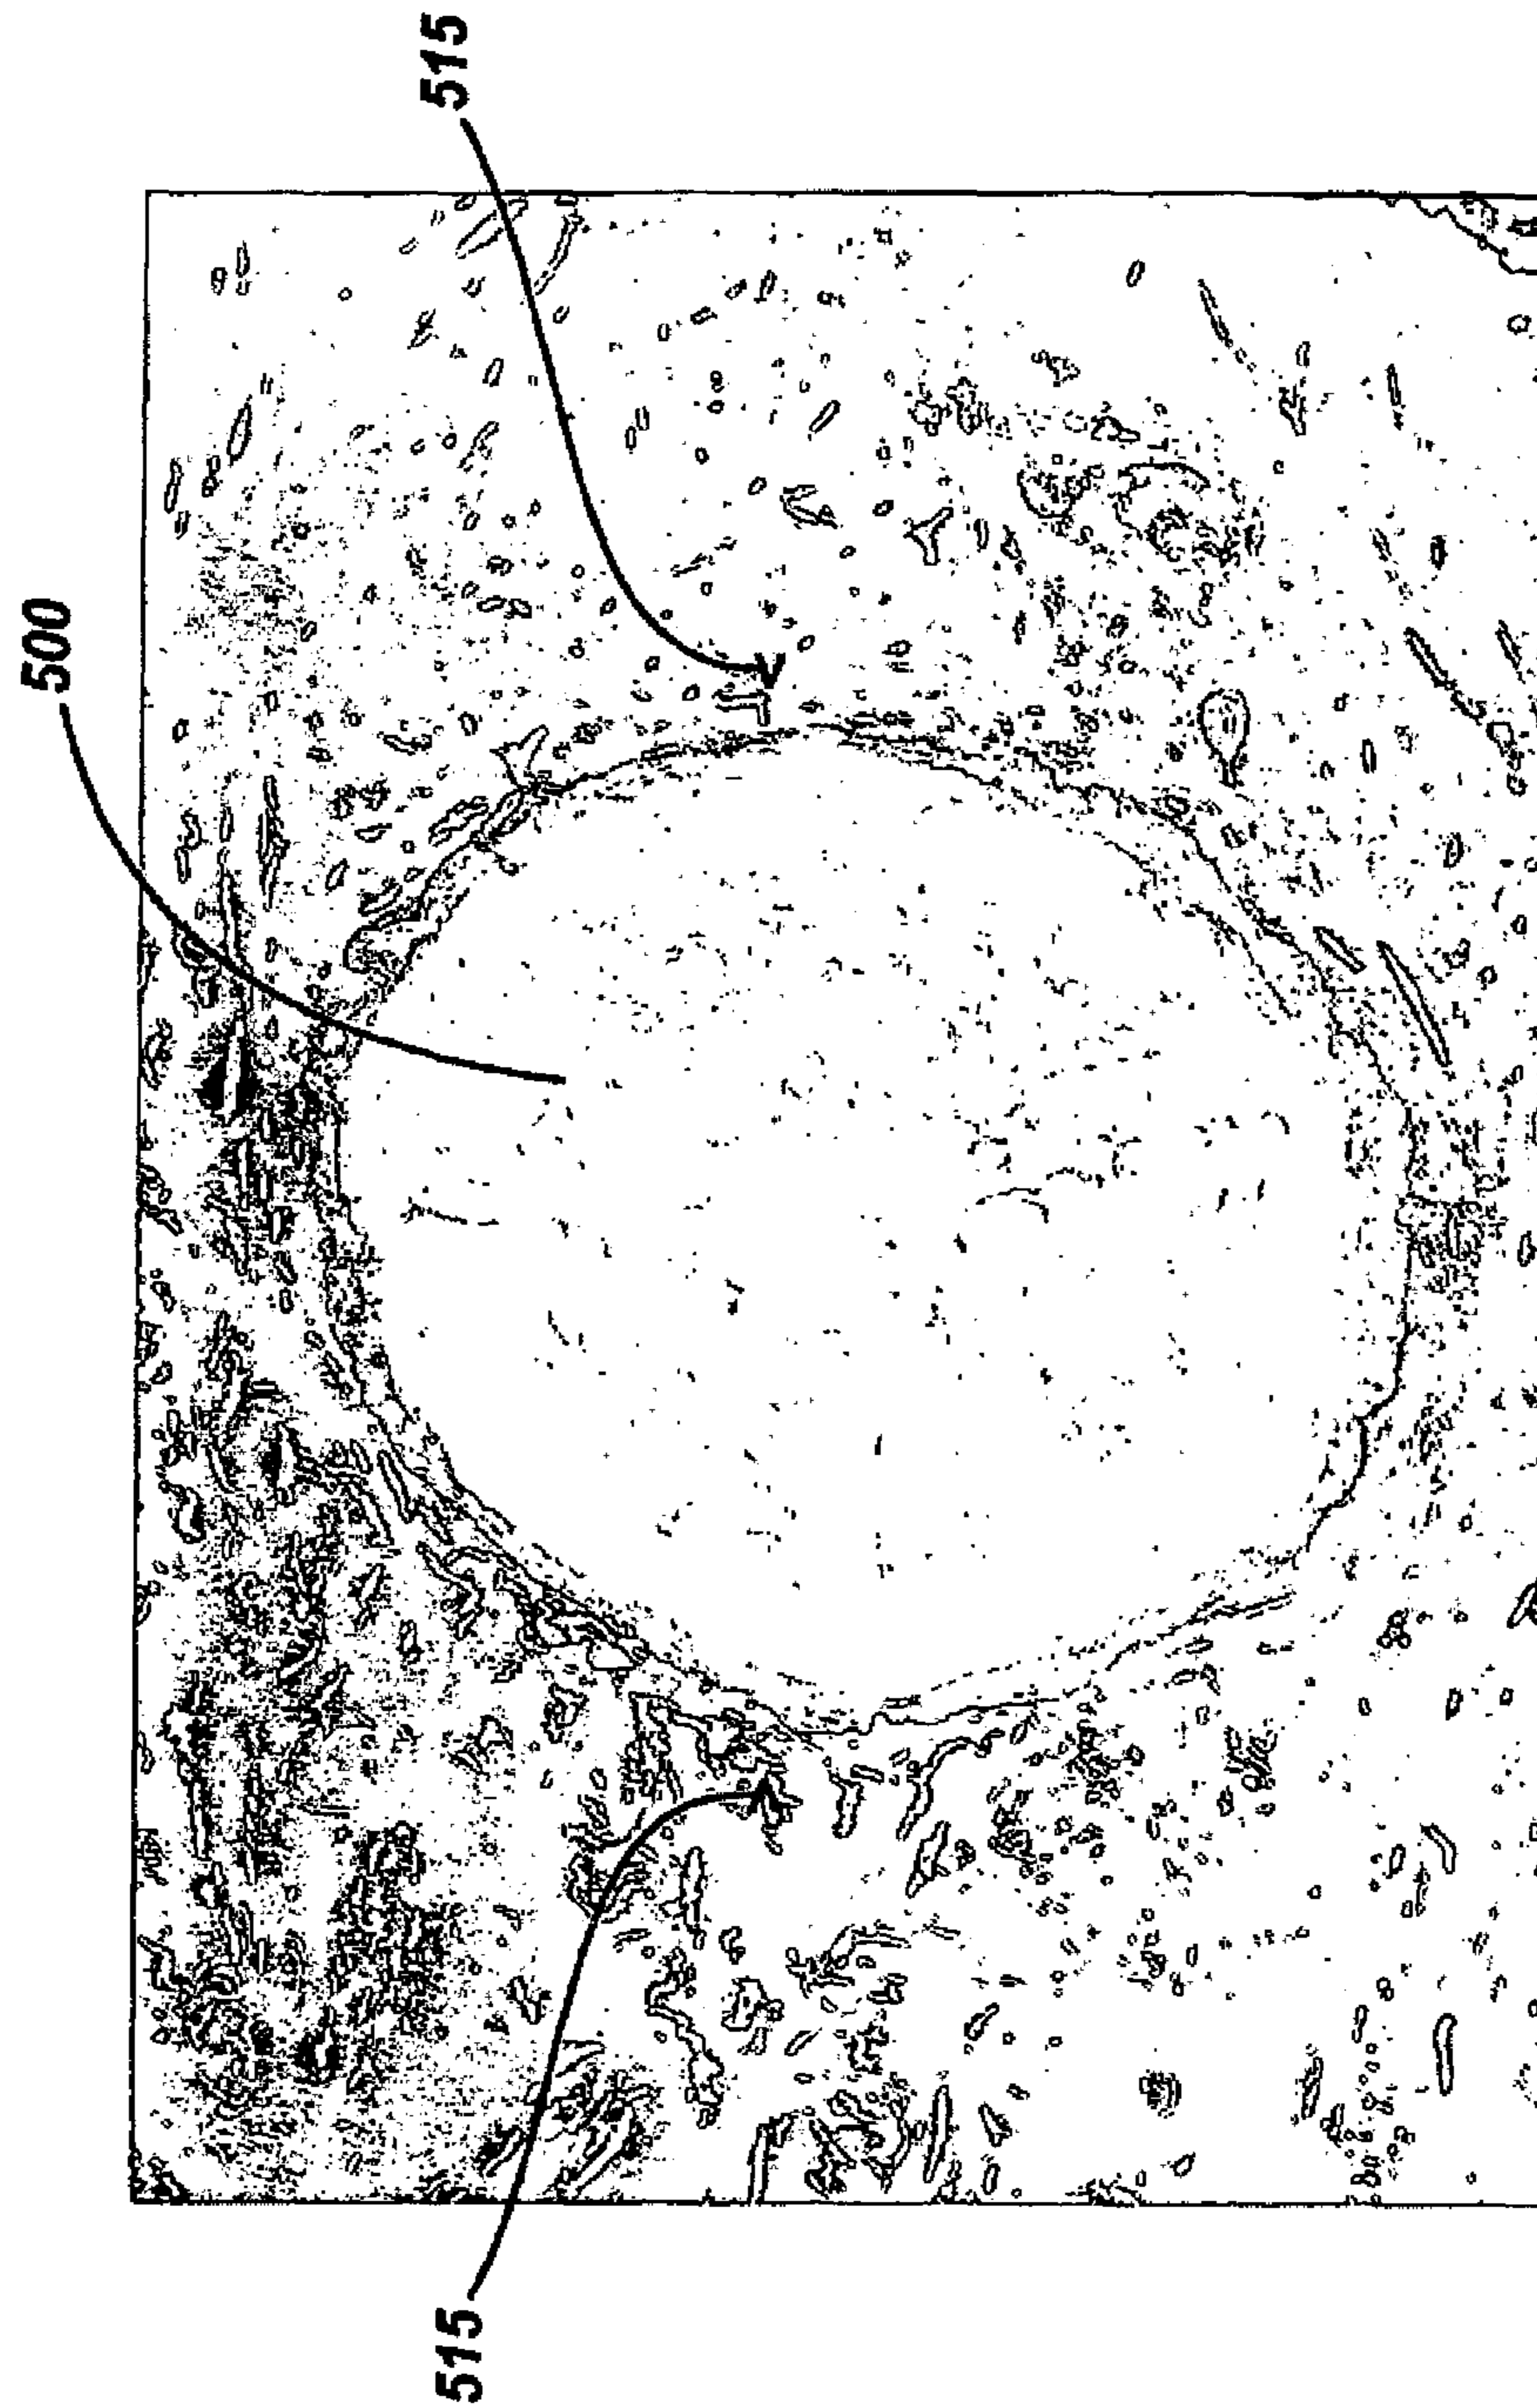

**Distance between arrows ~3mm**


**FIG. 11C**

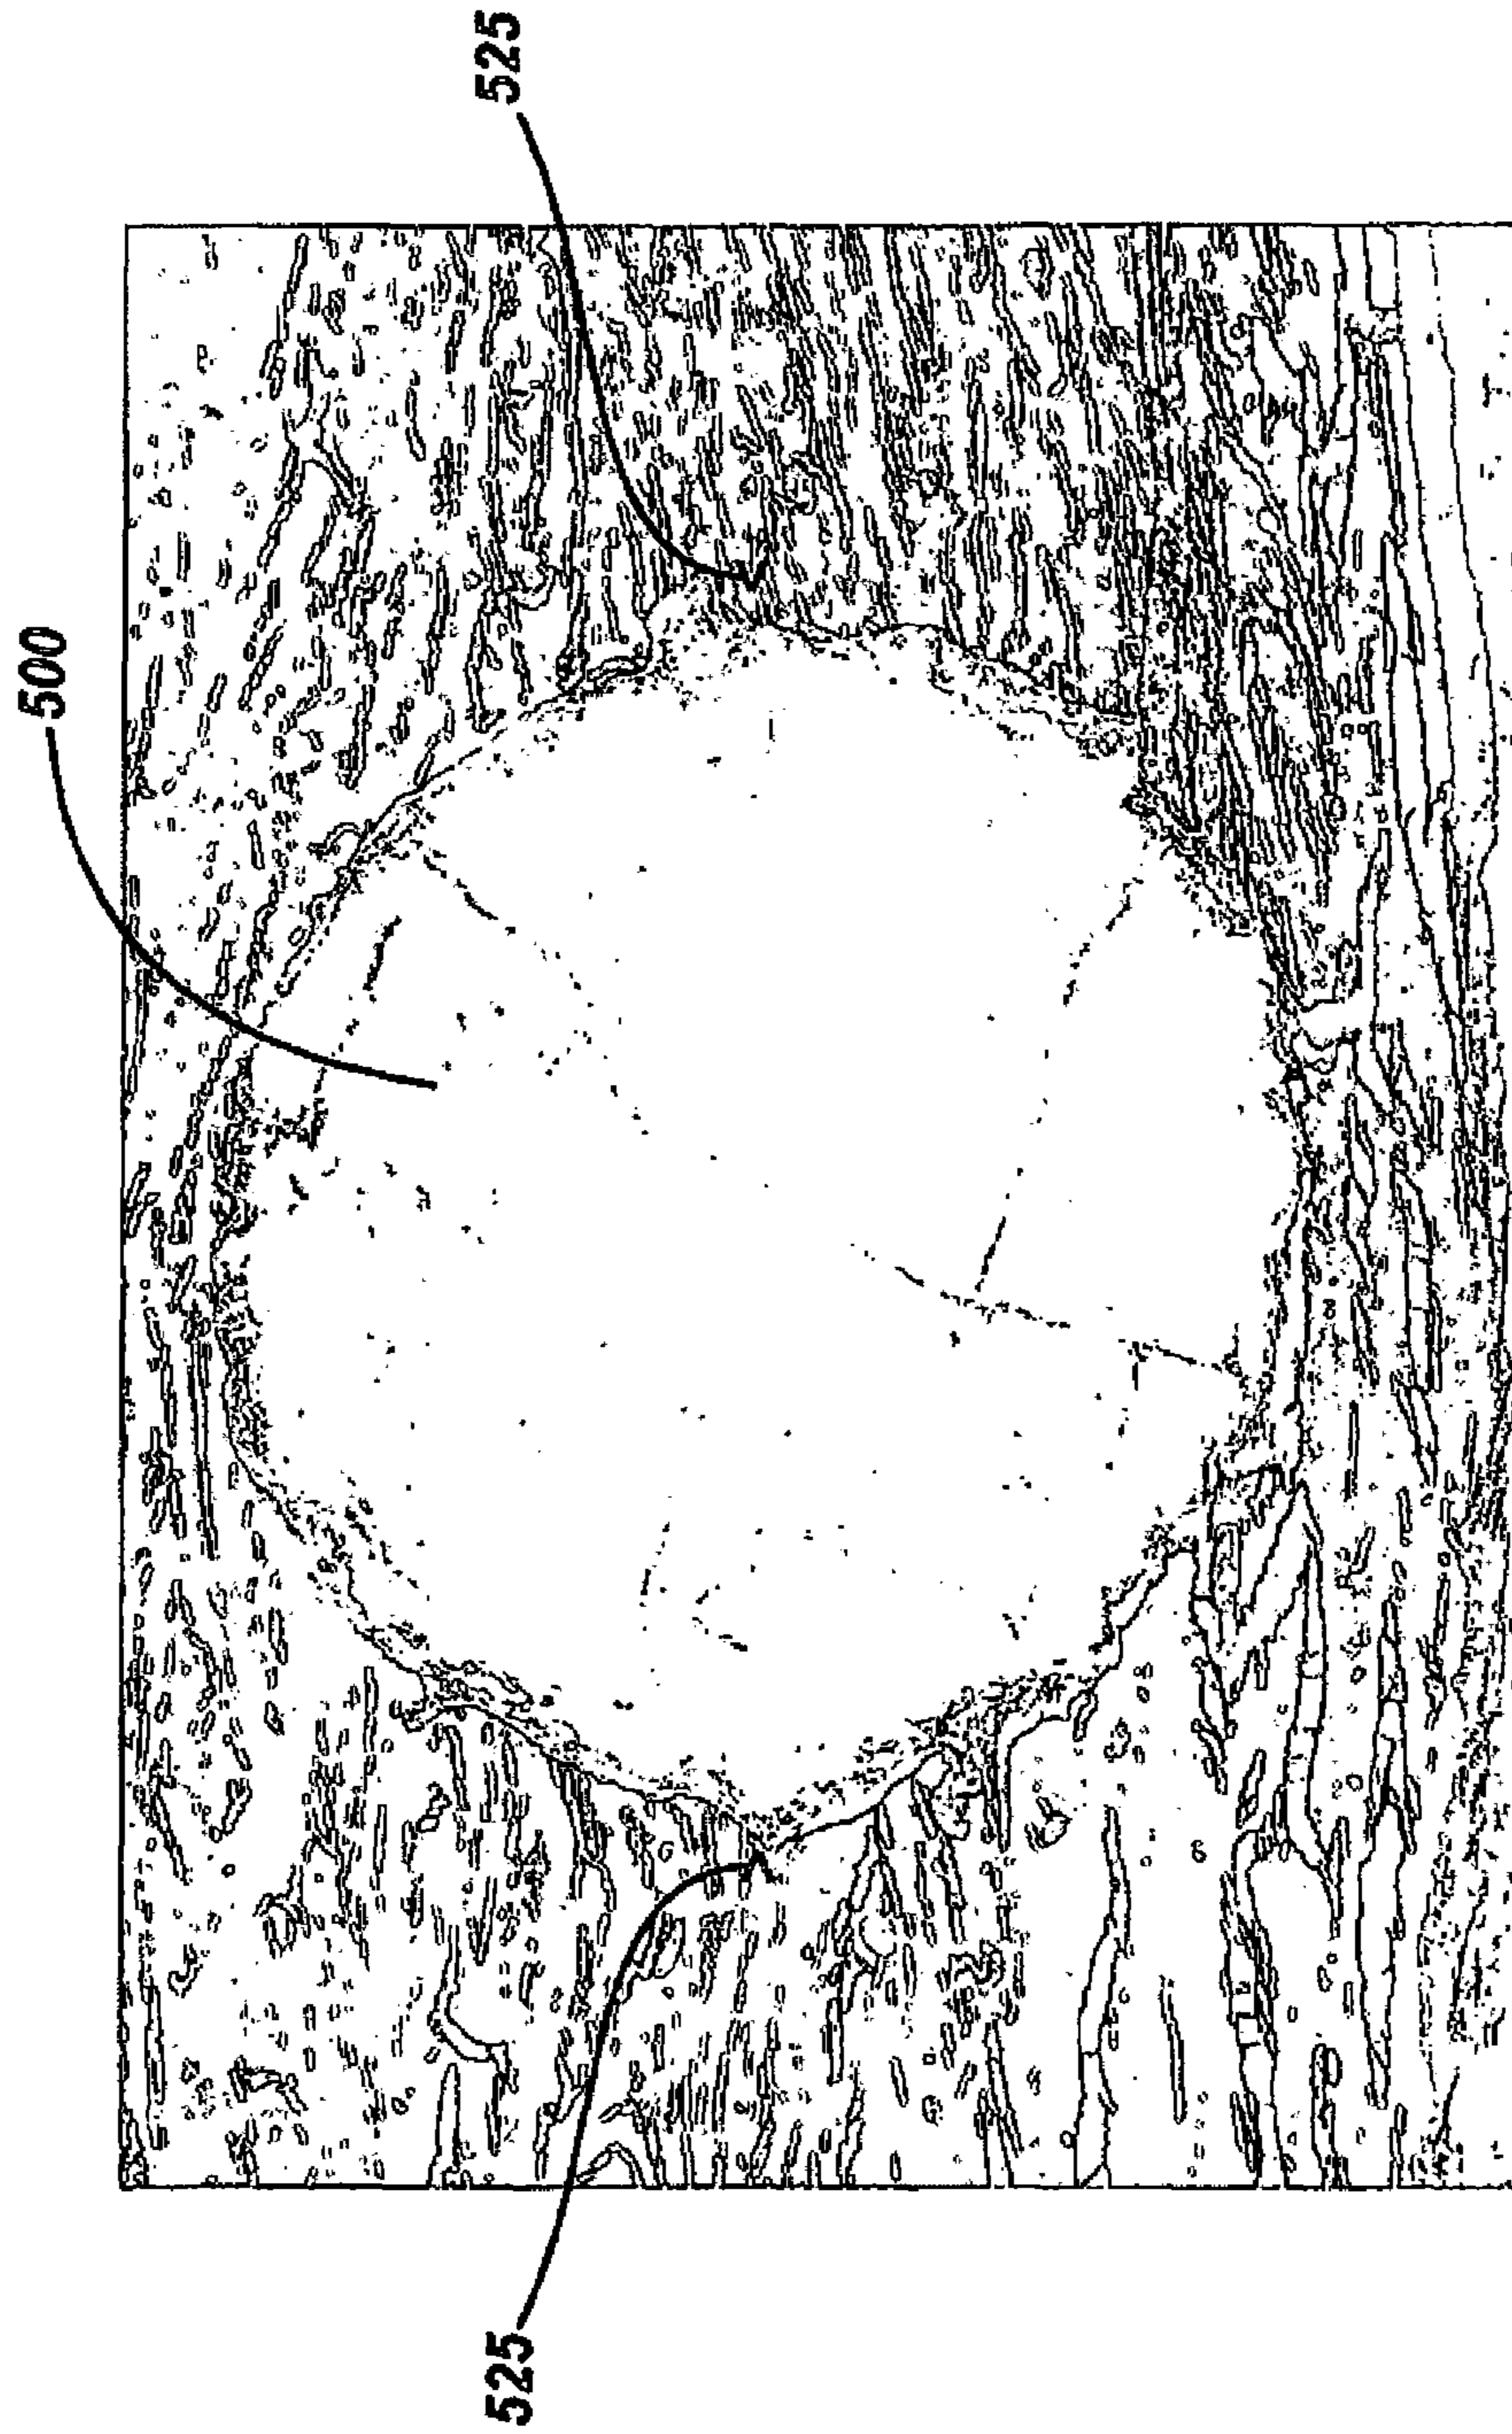

**Distance between arrows ~3.5mm**




**FIG. 11D**

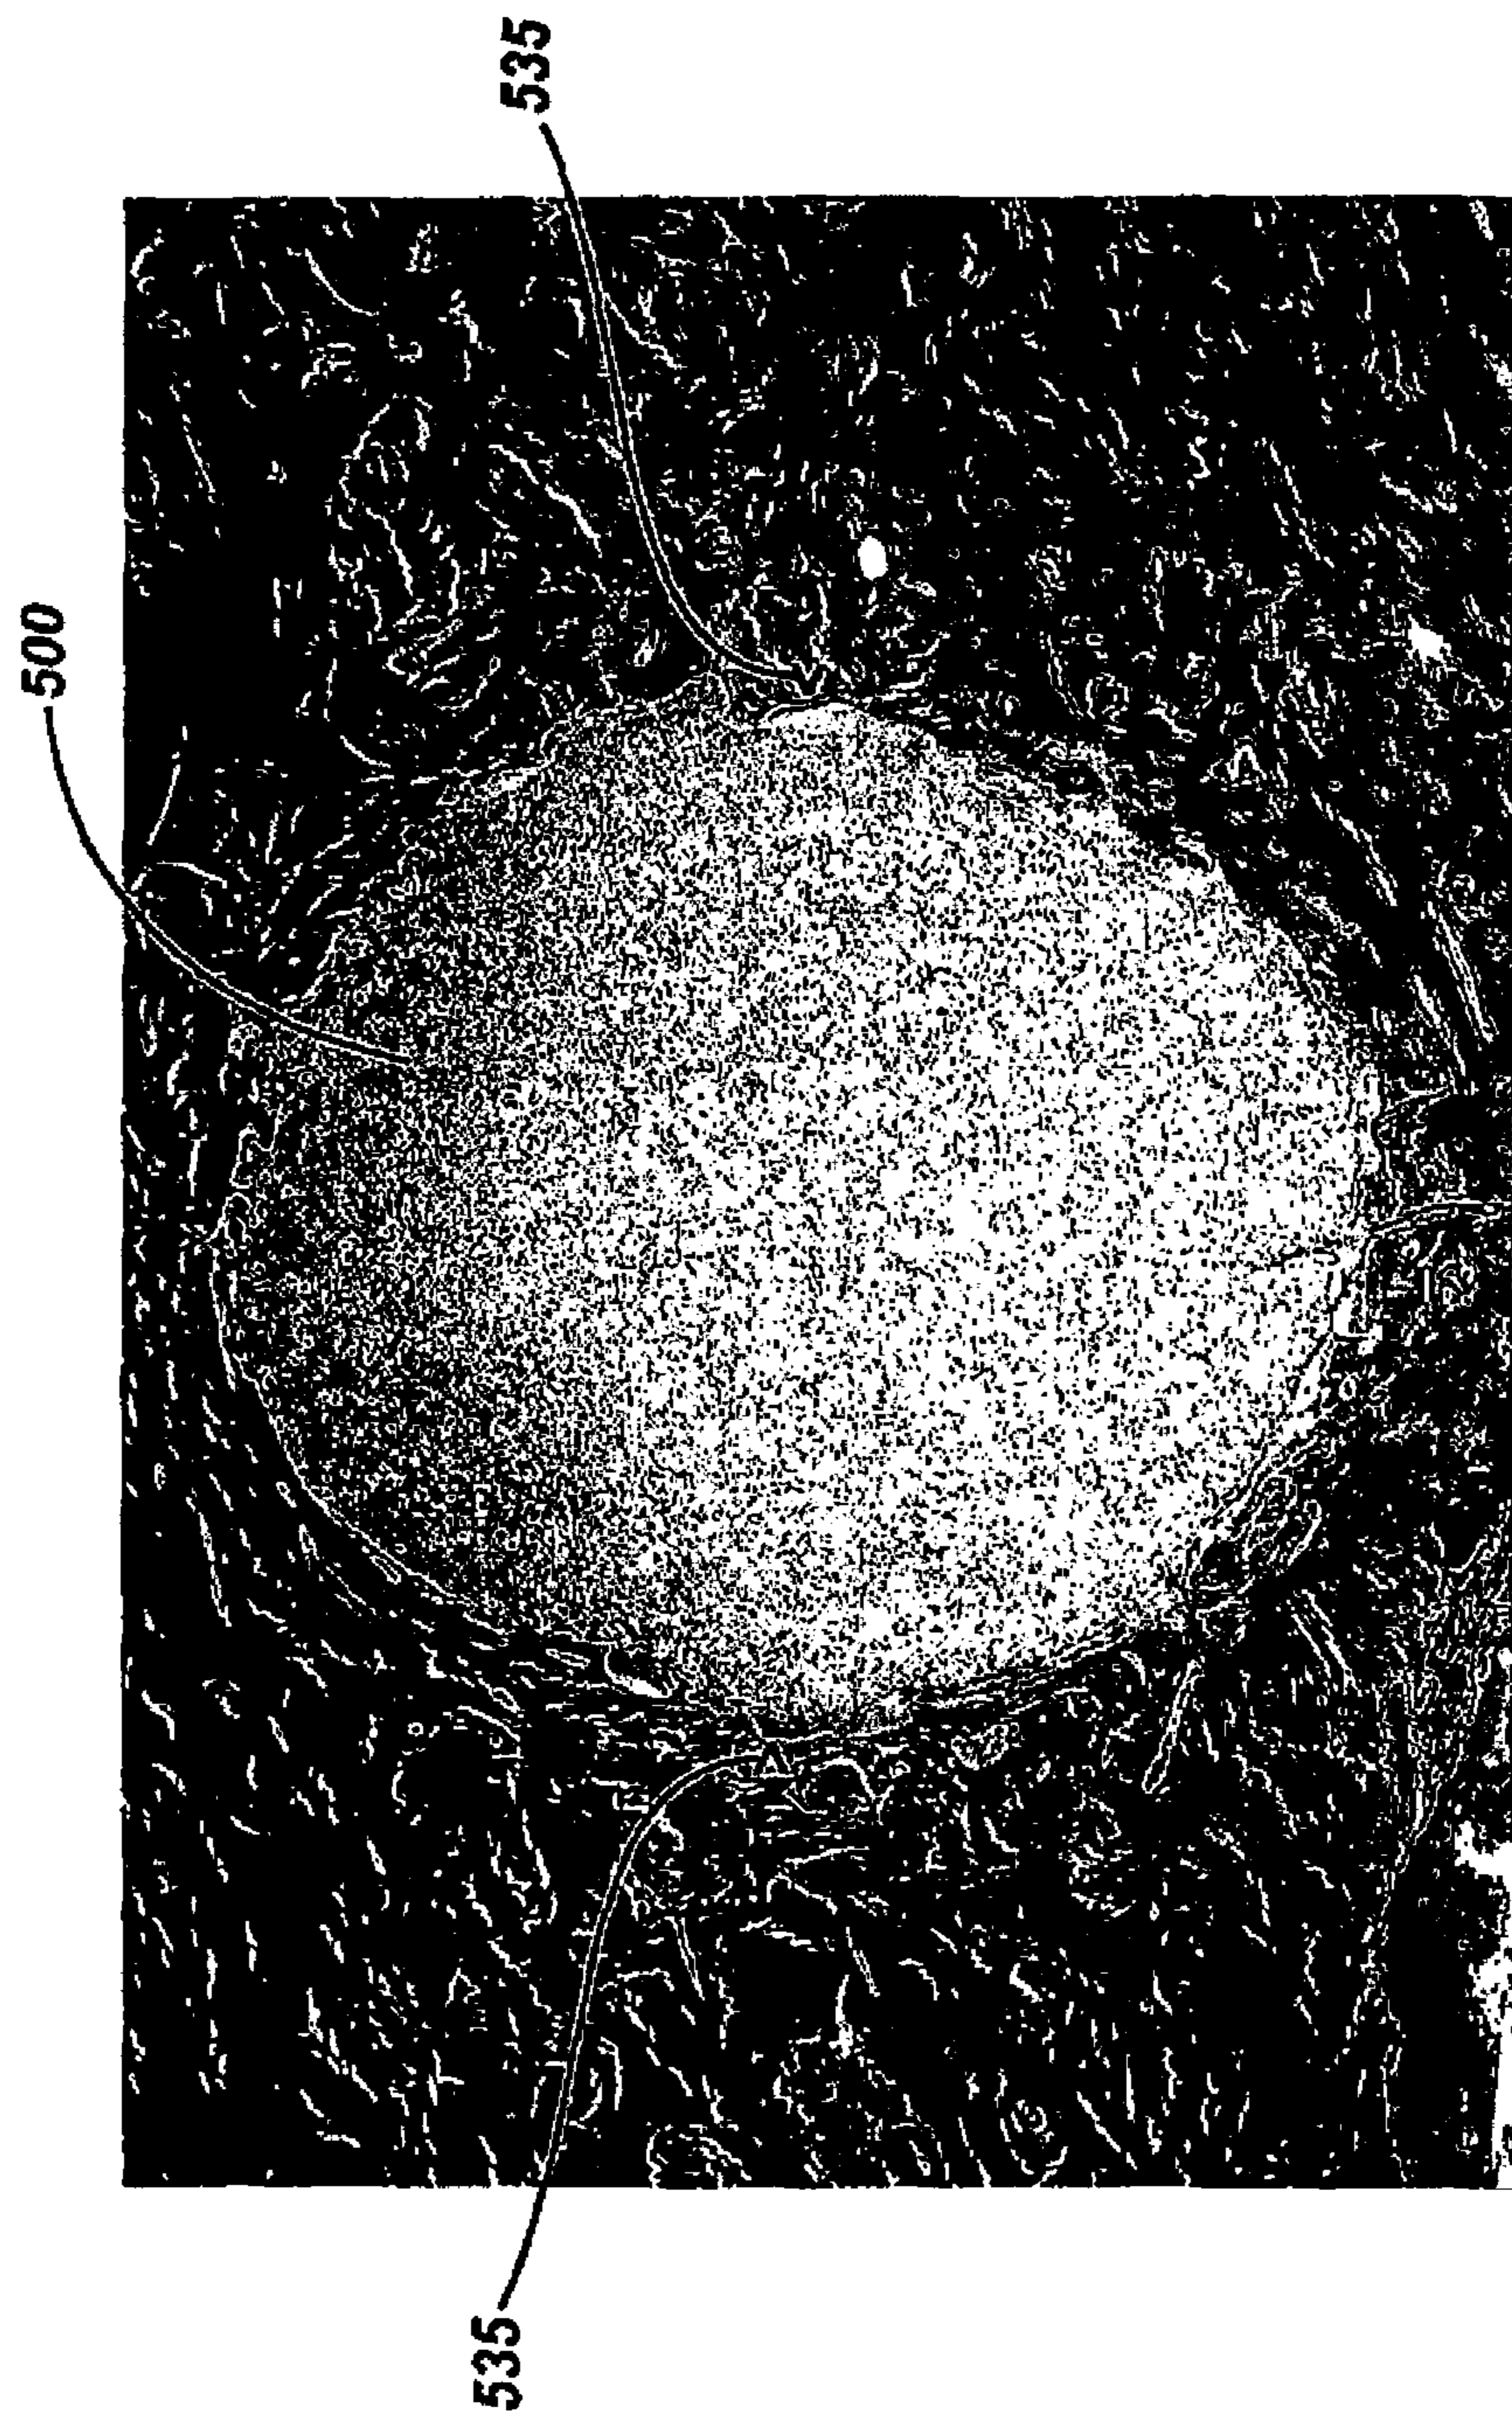

Distance between arrows ~3mm



**FIG. 11E**

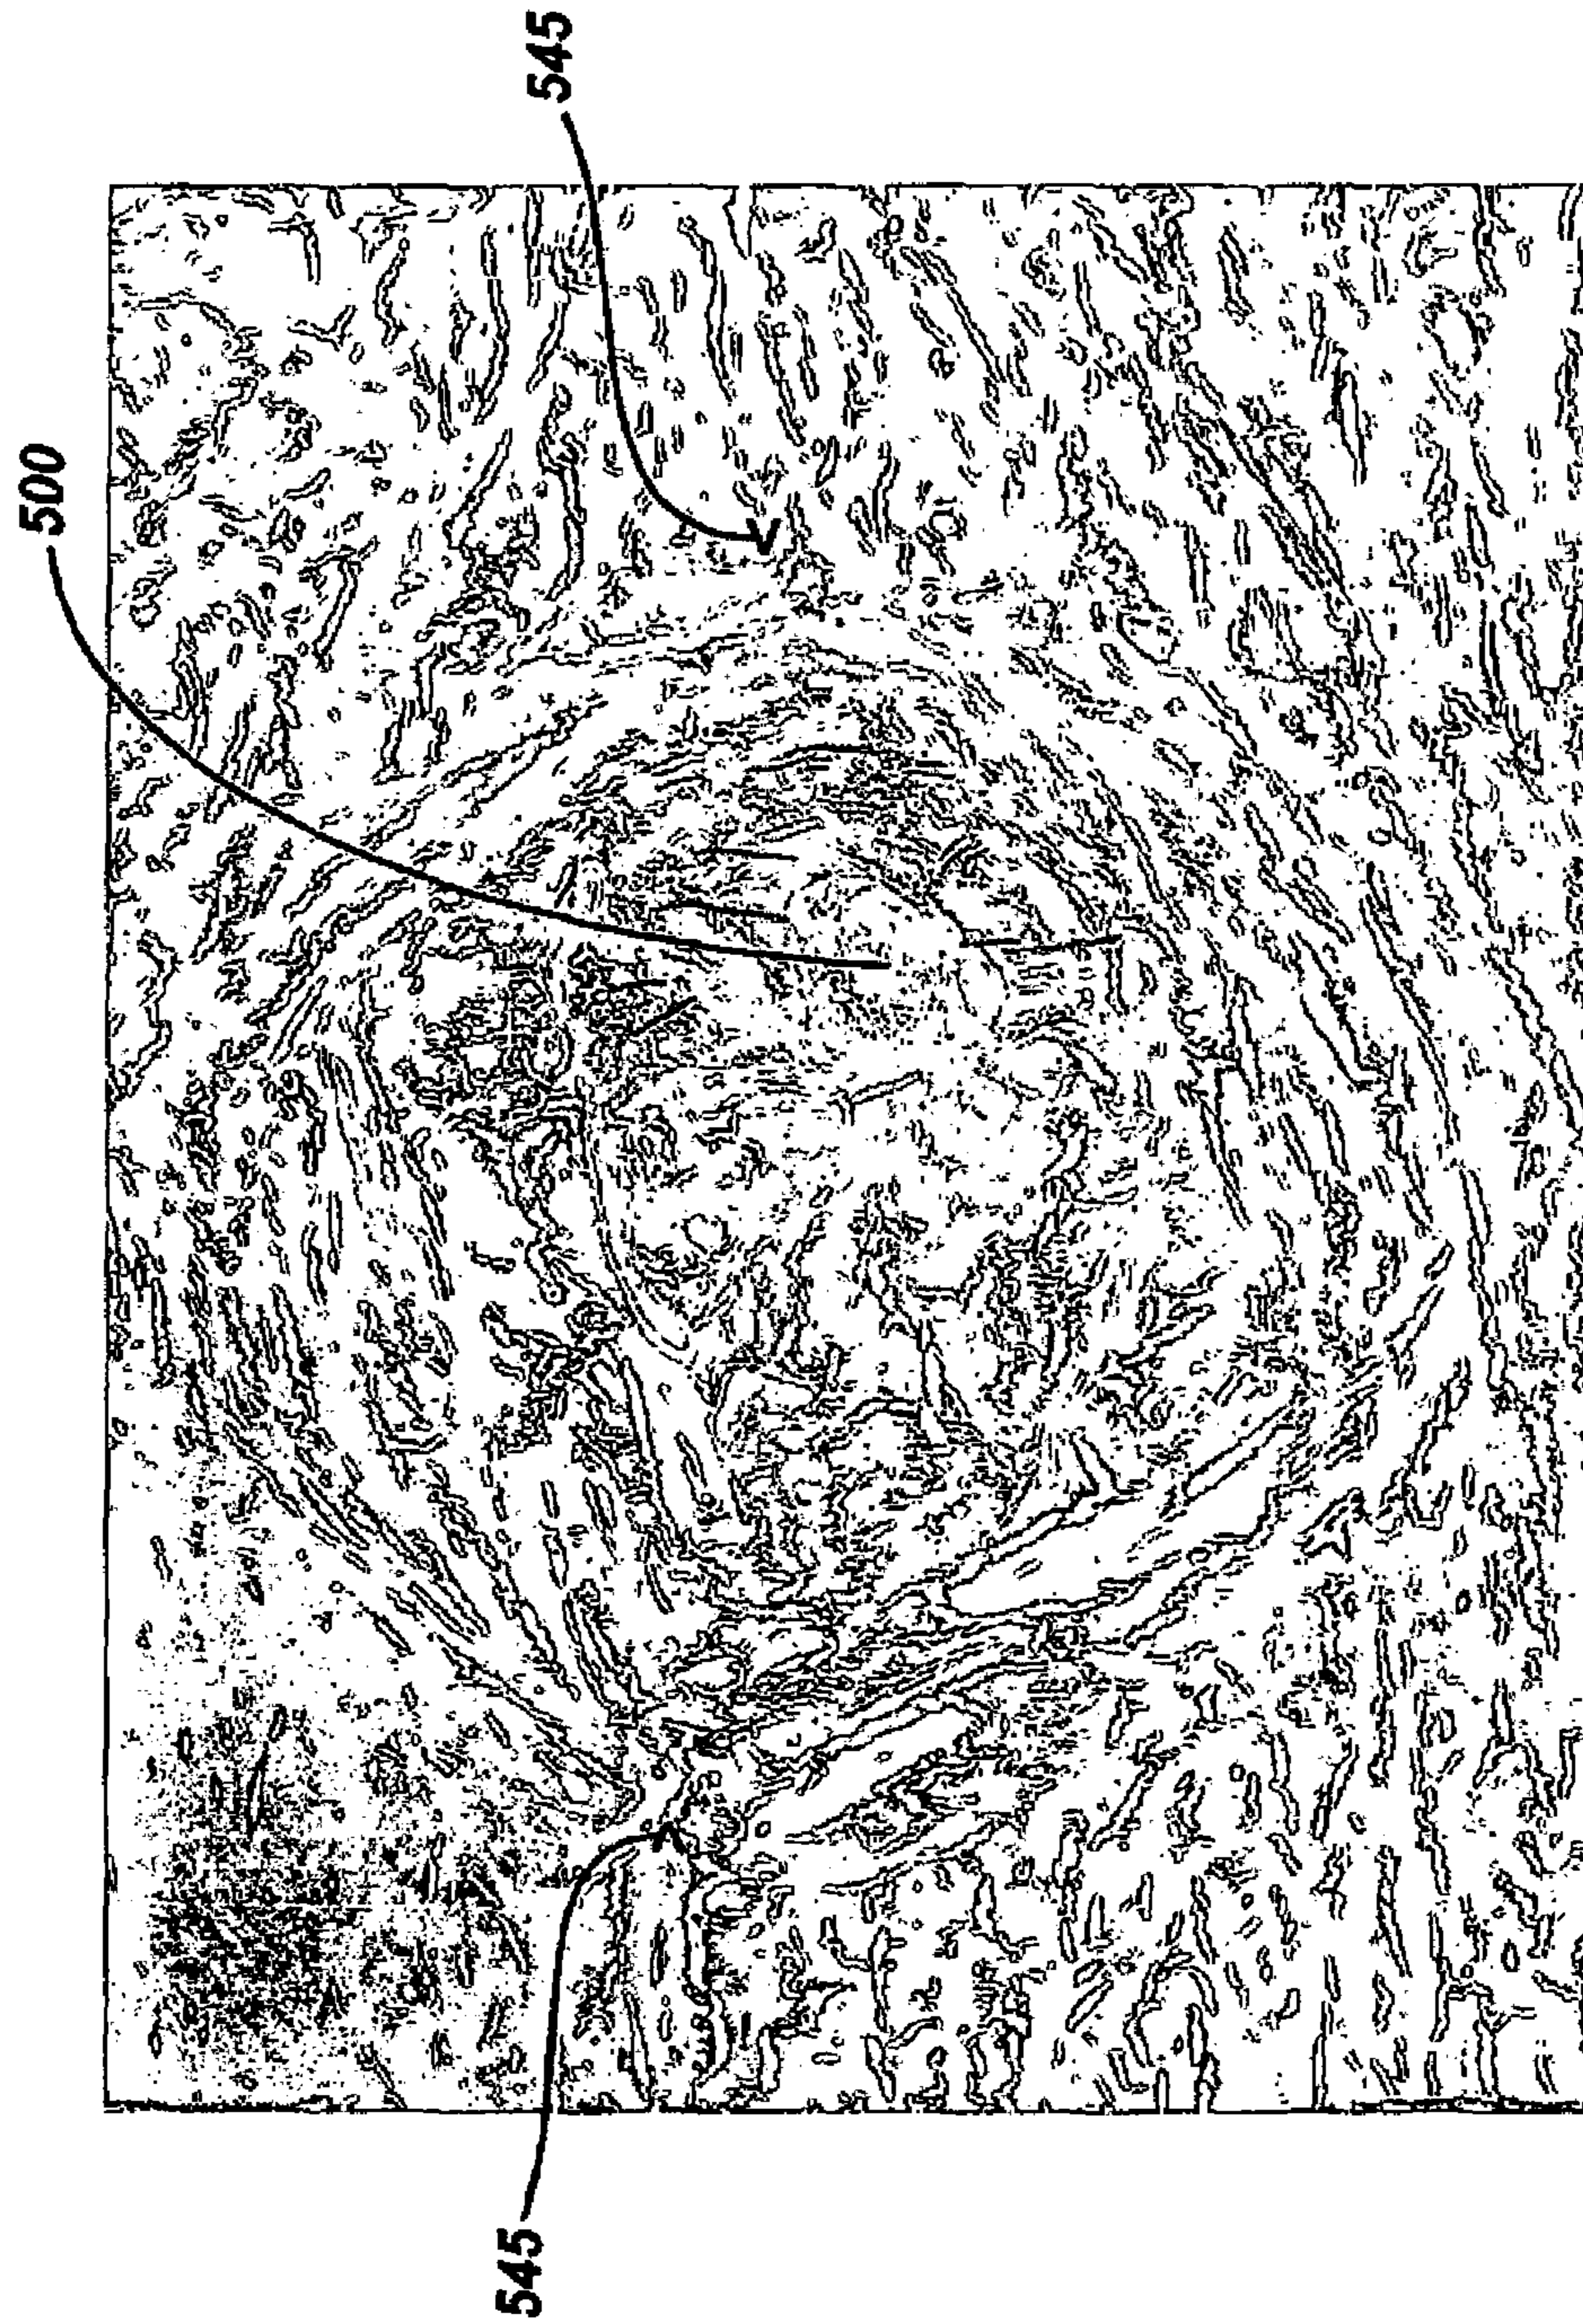

**Distance between arrows ~3.5mm**



1

**METHOD OF PERFORMING ANTERIOR  
CRUCIATE LIGAMENT RECONSTRUCTION  
USING BIODEGRADABLE INTERFERENCE  
SCREW**

CROSS REFERENCE TO RELATED  
APPLICATIONS

The present application is a continuation of U.S. patent application Ser. No. 10/673,737 filed on Sep. 29, 2003 now U.S. Pat. No. 8,016,865 and entitled "Method Of Performing Anterior Cruciate Ligament Reconstruction Using Biodegradable Interference Screw," which is hereby incorporated by reference in its entirety.

FIELD

The field of art to which this invention relates is surgical procedures for the repair of an anterior cruciate ligament, more specifically, a surgical procedure for affixing an anterior cruciate ligament graft into a bone using a biodegradable interference screw.

BACKGROUND

The knee joint is one of the strongest joints in the body because of the powerful ligaments that bind the femur and tibia together. Although the structure of the knee provides one of the strongest joints of the body, the knee may be one of the most frequently injured joints, e.g., athletes frequently stress and tear knee ligaments. The large number of ligament injuries has given rise to considerable innovative surgical procedures and devices for replacing and reconstructing torn or dislocated ligaments, typically involving grafting autografts, allografts, or a synthetic construct, to the site of a torn or dislocated ligament. For example, the replacement of an anterior cruciate ligament (ACL) may involve transplanting a portion of the patellar tendon, looped together portions of semitendinosus-gracilis (hamstring) tendons, or donor Achilles tendons, to attachment sites in the region of the knee joint.

Tears or ruptures of an anterior cruciate ligament of a knee (ACL) typically require a major surgical intervention wherein a replacement graft is mounted to the ends of the bones surrounding the knee in order to reconstruct the knee. A ruptured or damaged ACL typically results in serious symptoms such as knee instability resulting in diminished ability to perform high level or recreational sports, or in some cases daily activities relating to motility. Although the use of knee braces may alleviate some of these symptoms, the potential long term effects of a damaged ACL include meniscal damage and articular cartilage damage.

The basic steps in a conventional ACL reconstruction procedure include: harvesting a graft made from a portion of the patellar tendon with attached bone blocks; preparing the graft attachment site (e.g., drilling holes in opposing bones of the joint in which the graft will be placed); placing the graft in the graft attachment site; and rigidly fixing the bone blocks in place within the graft site, i.e., the holes or "bone tunnels". The screws used to fix the graft in place are called "interference screws" because they are wedged between the bone block and the wall of the bone tunnel into which the bone block fits. Typically, there is very little space between the bone block and the inner wall of the bone tunnel in the bone at the fixation site.

Several types of surgical procedures have been developed to replace the ACL. Although repair would be a preferred procedure, it is not typically possible since the end of the torn

2

ACL is typically not of sufficient length to reattach successfully. However, reconstructions can be made to a damaged ACL.

There are several types of conventional replacement grafts that may be used in these replacement procedures. In all procedures tibial and femoral tunnels are drilled by the surgeon using conventional techniques. Known, conventional drill guides and drills are used. In one type of procedure known as a bone-tendon-bone procedure, an autograft tendon is harvested from the patellar tendon along with an attached bone block on one end harvested from the patella and a harvested bone block on the other end harvested from the tibia. In order to secure the graft in the knee, one end is mounted into the tibial tunnel and other end is mounted into the femoral tunnel. This is done by mounting the opposed bone blocks in the tibial and femoral tunnels, respectively, in the following manner. A guide pin is passed through the tibial tunnel, into the femoral tunnel and out through the lateral femoral cortex. Suture is used to attach the graft to the proximal end of the guide pin. The distal end of the guide pin is then pulled out of the lateral cortex of the femur and the graft is pulled into the knee (femoral and tibial tunnels). Once the bone blocks are emplaced in the respective tibial and femoral tunnels, the blocks are secured in place in the following manner. One method of securing or fixing the ends of the graft in the tunnels is to use a conventional metallic interference screw. The screw is inserted into the opening of a tunnel and placed in between the graft and the interior surface of the bone tunnel. It is then turned and screwed into the tunnels, thereby forcing the end of the graft against an interior surface of the bone tunnel. The ends of graft are secured and maintained in place in the tunnel by means of a force fit provided by the interference screw.

Another surgical procedure for the replacement of an anterior cruciate ligament involves providing a graft ligament without attached bone blocks. The graft can be an autograft or an allograft. The autografts that are used may typically be harvested from the hamstring tendons or the quadriceps tendons. The allografts that are conventionally used are harvested from cadaveric sources, and may include the hamstring tendons, quadriceps tendons Achilles tendon, and tibialis tendons. If desired, and if readily available, it may be possible to use synthetic grafts or xenografts. Tibial and femoral tunnels are similarly drilled in the tibia and femur respectively using conventional techniques, drill guides and drills. Once the tunnels have been drilled, the surgeon then pulls the graft through the tibial and femoral tunnels using conventional techniques such that one end of the graft resides in the tibial tunnel and the other end of the graft resides in the femoral tunnel. For example, one conventional technique for pulling a graft through the tunnels is to attach the graft to the proximal end of a guide pin using conventional surgical suture. The guide pin is then passed through the tibial tunnel, into the femoral tunnel, and out through the femoral cortex. The distal end of the guide pin is then pulled out of the lateral cortex of the femur and the graft is pulled into the knee (femoral and tibial tunnels). After the surgeon has emplaced and positioned the ends of the graft in the respective tunnels, the graft ends need to be secured and fixed in place to complete the replacement procedure. One method of securing or fixing the ends of the graft in the tunnels is to use a conventional metallic interference screw. The screw is inserted into the opening of a tunnel and placed in between the graft and the interior surface of the bone tunnel. It is then turned and screwed into the tunnels, thereby forcing the end of the graft against an interior surface of the bone tunnel. The ends of the



graft are secured and maintained in place in the tunnel by means of a force fit provided by the bone screw.

Interference screws for anchoring ligaments to bone are typically fabricated from medically approved metallic materials that are not naturally degraded by the body. One potential disadvantage of such screws is that once healing is complete, the screw remains in the bone. An additional disadvantage of a metal screw is that in the event of a subsequent rupture or tear of the graft, it may be necessary to remove the metal screw from the bone site. Metallic screws may include a threaded shank joined to an enlarged head having a transverse slot or hexagonal socket formed therein to engage, respectively, a similarly configured, single blade or hexagonal rotatable driver for turning the screw into the bone. The enlarged heads on such screws can protrude from the bone tunnel and can cause chronic irritation and inflammation of surrounding body tissue.

Permanent metallic medical screws in movable joints can, in certain instances, cause abrading of ligaments during normal motion of the joint. Screws occasionally back out after insertion, protruding into surrounding tissue and causing discomfort. Furthermore, permanent metallic screws and fixation devices may shield the bone from beneficial stresses after healing. It has been shown that moderate periodic stress on bone tissue, such as the stress produced by exercise, helps to prevent decalcification of the bone. Under some conditions, the stress shielding which results from the long term use of metal bone fixation devices can lead to osteoporosis.

Biodegradable interference screws have been proposed to avoid the necessity of surgical removal after healing. Because the degradation of a biodegradable screw occurs over a period of time, support load is transferred gradually to the bone as it heals. This reduces potential stress shielding effects.

In order to overcome the disadvantages that may be associated with metal interference screws, interference screws made from biodegradable polymers are known in this art. For example, it is known to use an interference screw made from polylactic acid. Ideally, the biodegradable interference screw will rapidly absorb or break down and be replaced by bone. However, it is known that screws made from polylactic acid tend to maintain their structural integrity for very long periods of time thereby preventing the desired bone in growth. Attempts have been made to improve the bone regeneration process by using other biodegradable polymers and copolymers of lactic acid that resorb or absorb more quickly. The problem often associated with these quicker absorbing polymers or copolymers is that the bone regeneration may proceed at a much slower rate than the rate of resorption, resulting in premature mechanical failure of the screw and a resulting pull out of the graft end from the femoral tunnel. Some of the absorbable interference screws of the prior art may take several years to absorb, and may result in a fibrous tissue mass or cyst being left behind, not bone. This lack of bone in-growth may create fixation problems if the ACL is torn again, necessitating a new graft replacement. In addition, if the screw absorbs too slowly, the screw will need to be removed in the event of a subsequent failure of the graft.

Accordingly, what is needed in this art is a novel method of performing an ACL replacement graft procedure using a novel interference screw made from a biodegradable material which rapidly absorbs or degrades and promotes bone in-growth.

#### SUMMARY

Therefore, it is an object of the present invention to provide a novel method of replacing a ruptured or injured anterior

cruciate ligament with a graft using a novel biodegradable interference screw consisting of a composite of a biodegradable polymer and a biodegradable ceramic or bioglass.

Accordingly, a novel method of repairing an anterior cruciate ligament in the knee is disclosed. A replacement graft is provided having a first end and a second end. A bone tunnel is drilled in the tibia. A bone tunnel is also drilled in the femur. The first end of the graft is mounted in the femoral bone tunnel. The second end of the graft is mounted in the tibial bone tunnel. A biodegradable, composite interference screw is provided. The interference screw is made from a copolymer of poly (lactic acid) and poly(glycolic acid) and a bioceramic. The biodegradable screw is inserted into the femoral bone tunnel between an interior surface of the femoral bone tunnel and the first end of the graft. The interference screw is rotated such that the screw is substantially contained within the femoral bone tunnel, and the first end of the graft is fixed in place between the interference screw and a section of the interior surface of the femoral bone tunnel.

These and other features, aspects and advantages of the present invention will become more apparent from the following description and accompanying drawings.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The invention will be more fully understood from the following detailed description taken in conjunction with the accompanying drawings, in which:

FIG. 1A is a side view of a biodegradable interference bone screw useful in the method of the present invention.

FIG. 1B is an end view of the interference bone screw of FIG. 1A.

FIG. 1C is a cross-sectional view of the inference bone screw of FIG. 1B taken along view line A-A.

FIG. 2 is a side view of a driver device useful for emplacing the bone screw of FIG. 1 in a bone tunnel.

FIG. 3 illustrates a bone-tendon-bone graft prior to emplacement in a knee for an ACL reconstruction.

FIG. 4 shows a guide wire placed into the femoral tunnel between the tunnel wall and the bone block.

FIG. 5 illustrates a conventional tap being used to tap a hole between the wall and the bone block.

FIG. 6 shows a biodegradable interference screw being inserted into the femoral tunnel between the tunnel wall and the bone block.

FIG. 7 illustrates a guide wire placed into the tibial tunnel between the tunnel wall and the bone block.

FIG. 8. illustrates a conventional tap device being used to tap a hole between the tunnel wall and the bone block.

FIG. 9 illustrates the screw being inserted into the tibial tunnel between the tunnel wall and the bone block.

FIG. 10 is a side view of the knee after the ACL replacement procedure has been completed.

FIG. 11A is a histological section of a PLA/PGA bone pin containing [beta]-tricalcium phosphate and surrounding tissue.

FIG. 11B is a histological section of a PLA bone pin and surrounding tissue.

FIG. 11C is a histological section of a PLA bone pin and surrounding tissue.

FIG. 11D is a histological section of a PLA bone pin containing [beta]-tricalcium phosphate and surrounding tissue.

FIG. 11E is a histological section of a PLA/PGA bone pin containing [beta]-tricalcium phosphate and surrounding tissue.



## 5

## DETAILED DESCRIPTION

The novel interference screws of the present invention are a composite of a biodegradable polymer or copolymer and a bioceramic. The term biodegradable as used herein is defined to mean materials that degrade in the body and then are either absorbed into or excreted from the body. The term bioceramic as defined herein is defined to mean ceramic and glass materials that are compatible with body tissue. The bioceramics are preferably biodegradable.

The biodegradable polymers that can be used to manufacture the composite screws used in the novel process of the present invention include biodegradable polymers selected from the group consisting of aliphatic polyesters, polyorthoesters, polyanhydrides, polycarbonates, polyurethanes, polyamides and polyalkylene oxides. Preferably, the biodegradable polymers are aliphatic polyester polymers and copolymers, and blends thereof. The aliphatic polyesters are typically synthesized in a ring opening polymerization. Suitable monomers include but are not limited to lactic acid, lactide (including L-, D-, meso and D, L mixtures), glycolic acid, glycolide, .epsilon.-caprolactone, p-dioxanone (1,4-dioxan-2-one), trimethylene carbonate (1,3-dioxan-2-one), .delta.-valerolactone, and combinations thereof. These monomers generally are polymerized in the presence of an organometallic catalyst and an initiator at elevated temperatures. The organometallic catalyst is preferably tin based, e.g., stannous octoate, and is present in the monomer mixture at a molar ratio of monomer to catalyst ranging from about 10,000/1 to about 100,000/1. The initiator is typically an alkanol (including diols and polyols), a glycol, a hydroxyacid, or an amine, and is present in the monomer mixture at a molar ratio of monomer to initiator ranging from about 100/1 to about 5000/1. The polymerization typically is carried out at a temperature range from about 80.degree. C. to about 240.degree. C., preferably from about 100.degree. C. to about 220.degree. C., until the desired molecular weight and viscosity are achieved. It is particularly preferred to use a copolymer of poly(lactic acid) and poly(glycolic acid). In particular, a copolymer of about 85 mole percent poly(lactic acid) and about 15 mole percent poly(glycolic acid).

The bioceramics that can be used in the composite screws used in the novel process of the present invention include ceramics comprising mono-, di-, tri-, [alpha]-tri-, [beta]-tri-, and tetra-calcium phosphate, hydroxyapatite, calcium sulfates, calcium oxides, calcium carbonates, magnesium calcium phosphates. It is particularly preferred to use a [beta]-tricalcium phosphate.

In addition to bioceramics, bioglasses may also be used in the composite screws. The bioglasses may include phosphate glasses and bioglasses.

The amount of the bioceramic or bioglass in the composite interference screw will be sufficient to effectively promote bone in-growth. Typically the amount will be about 2.0 Vol. % to about 25.0 Vol. %, and preferably about 15.0 Vol. %.

The composite, biodegradable interference screws useful in the present invention are manufactured in conventional extrusion and molding processes using conventional extruding and molding equipment. In a typical process, dry biodegradable polymer pellets and dry bioceramic or bioglass are metered into a conventional heated screw extruder. The materials are heated and blended in the extruder for a sufficiently effective residence time to provide a viscous composite having a uniform distribution of the particles of bioglass or bioceramic. Then the viscous composite is cooled and chopped to form pellets of the homogenous composite. The interference screws may be molded in a conventional injection

## 6

molder. In a typical injection molder, pellets of composite are fed into a barrel, passed through a heating zone to melt the polymer, then pushed forward through a nozzle and into the cavity of a chilled mold. After cooling, the mold is opened, and the part is ejected.

A biodegradable interference screw **5** of the present invention is seen in FIGS. 1A-C. The screw **5** is seen to have an elongate body **10** having a cannulated passage **20** there-through, with proximal socket opening **22** and distal opening **26**. The body **10** is seen to have a plurality of thread flights **30** extending from the outer surface **12**. The body **10** is seen to have distal end **14** and proximal end **16**. A driver **50** for inserting or emplacing the crew **5** in a bone tunnel is seen in FIG. 2. The driver **50** has an elongated rod member **60** having distal end **62** and proximal end **64**. Distal end **62** is seen to have a driver **63** extending therefrom having a hexagonal configuration for mating with socket **22**. The screw **5** is mounted to driver **50** by inserting the driver **63** of distal end **62** into the mating proximal socket end **22** of the passage **20**.

The biodegradable composite interference screws described herein are used in the novel ACL reconstruction procedure of the present invention in the following manner as illustrated if FIGS. 3-10. Prior to reconstructing the ACL using a bone-tendon-bone graft, a patient is prepared for surgery in a conventional manner. The patient's knee **100** is prepared for surgery in a conventional manner including swabbing the skin around the knee with a conventional antiseptic solution, and draping the knee. The knee **100** is then angulated by the surgeon in a conventional manner to facilitate the surgical procedure. The patient is then anesthetized in a conventional manner using conventional anesthetics, either general or local at the discretion of the surgeon. As seen in FIG. 1, the knee **100** is seen to have a femur **150** having a distal end **160** and a tibia **130** having a proximal end **140**. Proximal end **140** is seen to have a tibial plateau **141**. Extending from the distal end **160** of femur **150** are the femoral condyles **170** separated by notch **175**. For the sake of illustration, the tendons, cartilage, fascia, soft tissue and skin are not shown. The knee **100** is accessed by the surgeon using a conventional arthroscope that is inserted through a conventional cannula, that has been previously emplaced in the knee **100** in a conventional manner through an incision in the skin covering the knee **100**. A flow of sterile saline is initiated through channels in the arthroscope into the knee **100**. The stumps of the ACL are removed from the surfaces of the tibial plateau **141** and the chondryl notch **175** using conventional shavers that are inserted through the cannula. A bone-tendon-bone graft **200** is harvested and prepared by the surgeon in a conventional manner. The graft **200** is harvested by making an incision in the skin over the knee **100** down the anterior patella to the tibial. A conventional sagittal saw is then used to harvest the opposed bone plugs **220** that are connected by harvested patellar tendon segment **210**. The tendon segment **210** is cut from the patellar tendon in a conventional manner using a scalpel. If desired, a graft without bone blocks attached may also be used in the method of the present invention.

The procedure continues by mounting a conventional tibial drill guide (not shown) to the proximal end of the tibia **130**. A conventional guide pin **250** is inserted into the drill guide and mounted to a conventional surgical drill. The guide pin **250** is seen to have elongated body **252** having distal cutting end **254** and proximal end **255** with suture mounting opening **257**. The guide pin **250** is drilled into the front of the tibia **130** in a conventional manner until the distal end **254** exits out from the tibial plateau **141**. The drill guide is then removed from the tibia **130** and a conventional surgical reamer is placed over



the guide pin 250 and turned to ream out a tibial tunnel 280 having a passage 282, an inner tunnel wall 283, a top opening 284 out of the tibial plateau 141 and a bottom opening 286 out through the tibia 130. Then the reamer and the guide pin 250 are removed from the tibial tunnel 280 and a conventional femoral aimer device (not shown) is inserted into tibial tunnel 280 and manipulated until the distal end of the femoral aimer engages the appropriate location on the femoral notch 175. Then the guide pin 250 is inserted through a passage in the femoral aimer, and the guide pin 250 is mounted to a conventional surgical drill and drilled into the femoral notch such that the distal end exits out through the lateral side of the femur 150 and through the skin overlying that section of the femur 150. Next, the femoral aimer is removed from the knee 100 and a conventional surgical bone reamer is placed over the guide pin 250 and moved through the tibial tunnel 280, and a femoral tunnel 290 is drilled through the femur having a passage 292, an inner tunnel wall 293, an upper opening 294 out through the lateral side of the femur 130 and a bottom opening 296 out of the femoral notch 175. The reamer is then removed from the bone tunnel 290.

Referring to FIG. 3., the graft 200 is illustrated proximal to the knee 100 having the tibial tunnel 280 and femoral tunnel 290 drilled and reamed in the tibia 130 and femur 150, respectively. The guide pin 250 is seen to reside in the knee 100 with the elongated body 252 of guide pin 250 substantially contained within tibial tunnel 280 and femoral tunnel 290, with distal end 254 exiting out through opening 294 and proximal end 255 exiting out from opening 286. Next, the surgeon threads sutures 230 through the suture tunnels 222 in bone blocks 220. The suture through the top bone block 220 is also threaded through opening 257 of guide pin 250. The surgeon then pulls guide pin 250 distally such that the graft 200 is displaced into the knee 100 with upper bone graft 220 located in passage 292 of femoral tunnel 290 and lower bone block 220 located in passage 282 of tibial tunnel 280. An optional step of tapping the bone block and bone tunnel is illustrated in FIGS. 4 and 5. A guide wire 300 is seen to be inserted into femoral bone tunnel 290 between bone block 220 and inner tunnel wall 293. Then, a conventional cannulated bone tap 310 is inserted over guide wire 300. The bone tap 310 has elongated cannulated member 310, having a transverse handle 314 mounted to proximal end 312 and a tapping/cutting end 318 mounted to distal end 316. The tapping cutting end 318 is rotated by rotating handle 314, causing an opening to be cut and threads to be tapped between inner wall 293 and bone block 220 in the femoral tunnel 290. Then, as seen in FIG. 6, a biodegradable interference screw 5 mounted to a driver 50 is mounted to the guide wire 300 and threaded into the femoral tunnel 290 between the bone block 220 and the inner wall 293, thereby securing the upper bone block 220 in the passage 292 of femoral tunnel 290. The guide wire is then removed from the femoral tunnel 290 and inserted into opening 286 of and into passage 280 of tibial tunnel 280 between the lower bone block 220 and the inner wall 183 as seen in FIG. 7. Then, the surgeon tensions the graft 200 by pulling proximally on sutures 230 connected to lower bone block 220. Then, the bone tap 310 is inserted into tibial tunnel 280 over the guide wire 300 and an opening and threads are cut and tapped between inner wall 283, and bone block 220. Finally, the bone tap 310 is removed and as seen in FIG. 9, a biodegradable interference screw 5 is mounted over the guide wire 300 and threaded into the tibial tunnel 280 between inner wall 282 and lower bone block 220, thereby securing the lower bone block 220 in tibial tunnel 280. This completes the ACL reconstruction, and the graft 200 is now secured in the knee 100. The complete reconstructed knee 100 is seen in

FIG. 10. The surgeon then checks the knee for proper flexion and completes the procedure in a conventional manner by removing the scope and portal, and conventionally closing and/or suturing and bandaging all incisions.

The following examples are illustrative of the principles and practice of the present invention although not limited thereto.

#### EXAMPLE 1

Biodegradable composite bone pins 1 were prepared in a conventional manner and into the femurs of mammalian laboratory animals. The pins were of the following three compositions: A) composites of 15/85% by volume [beta]-tricalcium phosphate and (85/15) poly (lactide co-glycolide); B) poly(lactide); and C) composite of 15%/85% by volume [beta]-tricalcium phosphate and poly(lactide). About 24 months after implantation, the animals were euthanized and histological sections were obtained. As seen in FIG. 11A, a bone pin 500 having a Composition (A) demonstrated a significant degree of absorption when compared with the original diameter indicated by arrows 505, and significant tissue (bone) in-growth. In addition, minimal tissue reaction was observed. As seen in FIGS. 11B and 11C, bone pins 510 and 520 having Composition (B) exhibited minimal absorption compared with the original diameters indicated by arrows 515 and 525, respectively. As seen in FIG. 11D, a bone pin 530 having Composition C showed minimal absorption compared with the original diameter indicated by arrows 535. And, as seen in FIG. 11E, a bone pin 540 having Composition A demonstrated a significant degree of absorption compared with the original diameter indicated by arrows 545, and significant tissue (bone) in-growth. Minimal tissue reaction was observed.

The novel ACL graft replacement method of the present invention using a composite interference screw made from a bioabsorbable polymer and a bioceramic or bioglass has many advantages. The advantages include having improved bioabsorption and bone replacement, improved tissue in-growth, and minimizing tissue trauma. In addition, there is an optimal balance between stiffness and elasticity of the screws.

Although this invention has been shown and described with respect to detailed embodiments thereof, it will be understood by those skilled in the art that various changes in form and detail thereof may be made without departing from the spirit and scope of the claimed invention.

What is claimed is:

1. A method of replacing an anterior cruciate ligament in a knee, comprising:

inserting a biodegradable composite interference screw into a bone tunnel between an interior surface of the bone tunnel and a first end of a graft mounted within the bone tunnel, said interference screw comprising a biodegradable comprising a copolymer of poly (lactic acid) and poly(glycolic acid), and a bioceramic; and rotating the interference screw such that the screw is substantially contained within the bone tunnel, and the first end of the graft is fixed in place between the interference screw and a section of the interior surface of the bone tunnel; wherein the biodegradable, composite interference screw degrades in the body.

2. The method of claim 1, further comprising inserting a second end of the graft into a second bone tunnel and anchoring the second end of the graft within the second bone tunnel.

3. The method of claim 1, wherein the bioceramic comprises a bioceramic selected from the group consisting of



9

mono-, di-, tri, [alpha]-tri-, [beta]-tri and tetra-calcium phosphate, hydroxyapatite, calcium sulfates, calcium oxides, calcium carbonate, and magnesium calcium phosphates.

4. The method of claim 1, wherein the bioceramic comprises [beta]-tricalcium phosphate.

5. The method of claim 1, wherein the bioabsorbable polymer comprises a copolymer of polylactic acid and poly (glycolic acid) comprising about 85 mole percent to about 95 mole percent of poly (lactic acid) and about 5 mole percent to about 15 mole percent of poly (glycolic acid).

6. The method of claim 1, wherein the bioabsorbable polymer comprises a co-polymer of about 85 mole percent poly (lactic acid) and about 15 mole percent poly (glycolic acid).

7. The method of claim 1, wherein the composite screw comprises about 2.0 Volume percent to about 25.0 Volume percent of bioceramic.

8. The method of claim 1, wherein the composite screw comprises about 15.0 Volume percent of bioceramic.

10

9. The method of claim 1, wherein the graft has a bone block attached thereto.

10. The method of claim 1, further comprising tapping the inner surface of the bone tunnel to create a threaded space therein.

11. A biodegradable composite interference screw, comprising:

an elongate body having a cannulated passage extending therethrough between proximal and distal ends thereof such that the elongate body has a proximal opening and a distal opening, the elongate body having a thread formed on an outer surface thereof and extending between the proximal and distal ends, and the elongate body comprising a biodegradable polymer, and the biodegradable polymer comprising a copolymer of poly (lactic acid) and poly(glycolic acid), and a bioceramic, wherein the elongate body is configured to degrade when implanted in bone.

\* \* \* \* \*