



US008845681B2

(12) **United States Patent**  
**Grace**

(10) **Patent No.:** **US 8,845,681 B2**  
(45) **Date of Patent:** **\*Sep. 30, 2014**

(54) **RIGIDLY-LINKED ARTICULATING WRIST WITH DECOUPLED MOTION TRANSMISSION**

(58) **Field of Classification Search**  
USPC ..... 606/1, 130, 205, 208; 600/102; 74/490.03

See application file for complete search history.

(71) Applicant: **Kenneth Grace**, Knoxville, TN (US)

(72) Inventor: **Kenneth Grace**, Knoxville, TN (US)

(73) Assignee: **Intuitive Surgical Operations, Inc.**, Sunnyvale, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **13/633,963**

(22) Filed: **Oct. 3, 2012**

(65) **Prior Publication Data**

US 2013/0030449 A1 Jan. 31, 2013

**Related U.S. Application Data**

(60) Continuation of application No. 11/948,052, filed on Nov. 30, 2007, now Pat. No. 8,292,916, which is a division of application No. 10/013,170, filed on Jun. 7, 2002, now Pat. No. Re. 43,049, which is a continuation-in-part of application No. 09/262,134, filed on Mar. 3, 1999, now Pat. No. 6,436,107, which is a continuation-in-part of application No. 08/873,190, filed on Jun. 11, 1997, now Pat. No. 6,102,850, which is a continuation-in-part of application No. 08/755,063, filed on Nov. 22, 1996, now Pat. No. 5,855,583.

(51) **Int. Cl.**  
**A61B 17/00** (2006.01)

(52) **U.S. Cl.**  
USPC ..... **606/205; 74/490.03**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

977,825 A	12/1910	Murphy
1,327,577 A	1/1920	Turner
3,171,549 A	3/1965	Orloff
3,280,991 A	10/1966	Melton et al.
3,628,535 A	12/1971	Ostrowsky et al.
4,058,001 A	11/1977	Waxman
4,128,880 A	12/1978	Cray, Jr.
4,221,997 A	9/1980	Flemming
4,367,998 A	1/1983	Causer
4,401,852 A	8/1983	Noso et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

DE	9204118	7/1992
DE	9409979 U1	9/1994

(Continued)

**OTHER PUBLICATIONS**

EP Patent Application No. 08017470.9 Extended European Search Report, mailed Oct. 28, 2009, 6 pages.


(Continued)

*Primary Examiner* — Victor Nguyen

(57) **ABSTRACT**

The present invention is a device having a rigidly linked jaw that is decoupled from an articulating wrist. The device provides for articulating motion as well as actuation that may be used in grasping, cutting, suturing or the like.

**7 Claims, 3 Drawing Sheets**

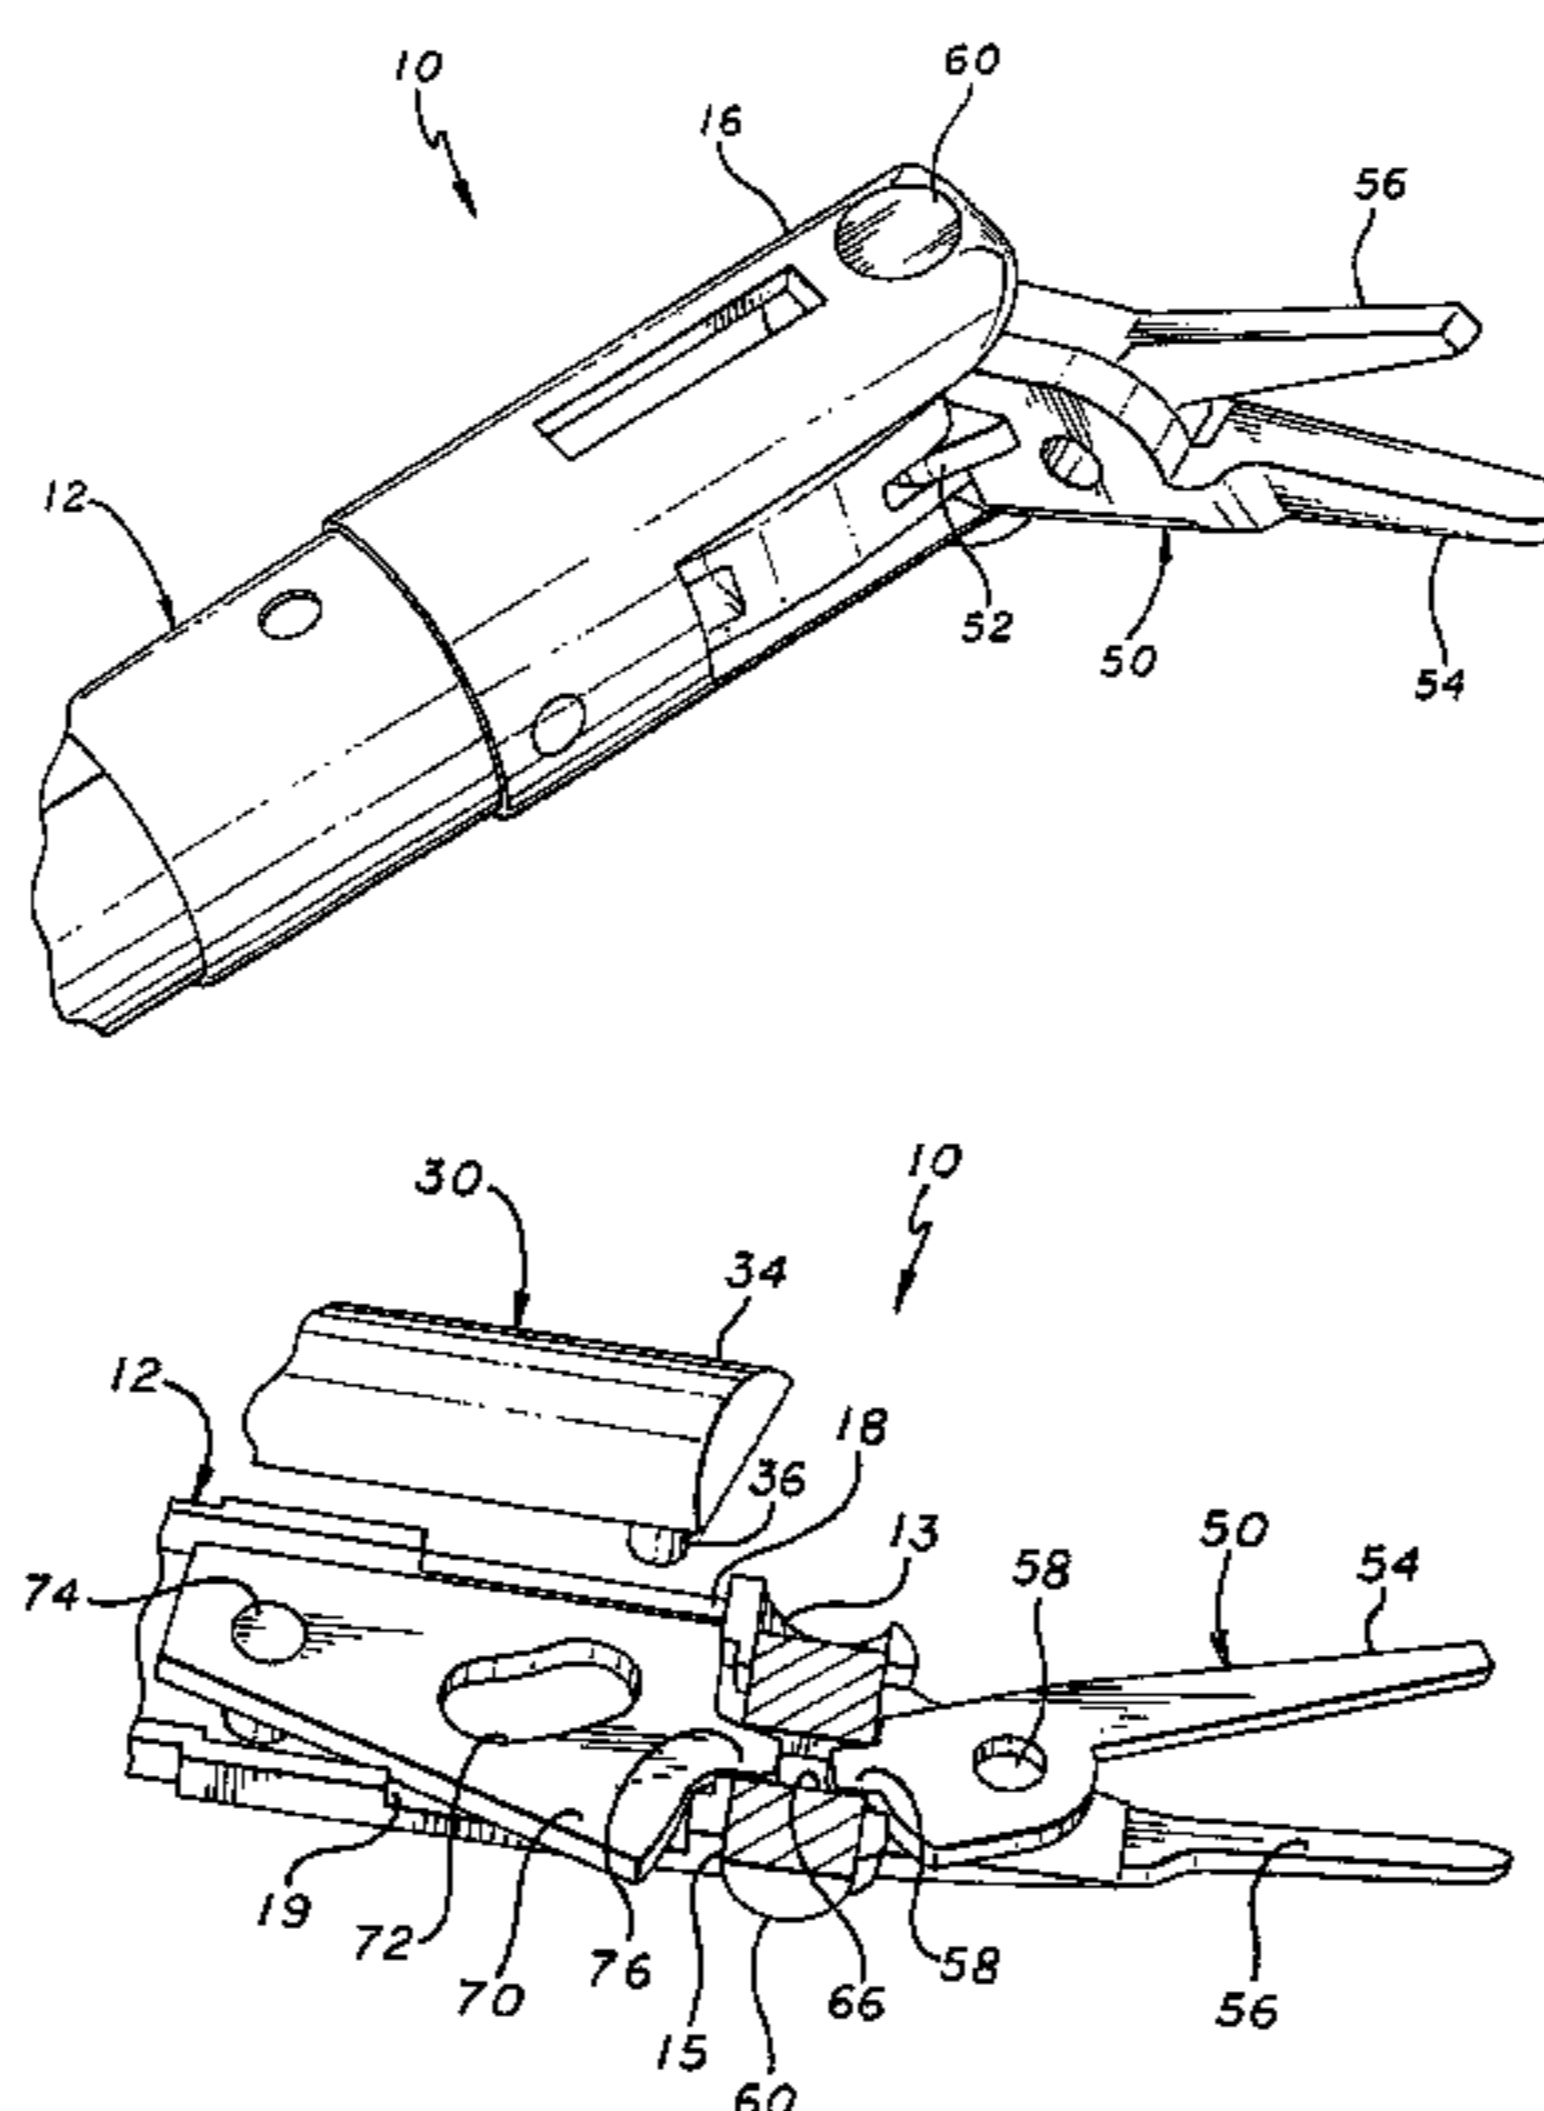

(56)

## References Cited

## U.S. PATENT DOCUMENTS

4,456,961 A	6/1984	Price et al.	5,271,384 A	12/1993	McEwen et al.
4,460,302 A	7/1984	Moreau et al.	5,275,608 A	1/1994	Forman et al.
4,474,174 A	10/1984	Petruzzi	5,279,309 A	1/1994	Taylor et al.
4,491,135 A	1/1985	Klein	5,282,806 A	2/1994	Haber et al.
4,503,854 A	3/1985	Jako	5,282,826 A	2/1994	Quadri
4,517,963 A	5/1985	Michel	5,289,273 A	2/1994	Lang
4,523,884 A	6/1985	Clement et al.	5,289,365 A	2/1994	Caldwell et al.
4,586,398 A	5/1986	Yindra	5,299,288 A	3/1994	Glassman et al.
4,604,016 A	8/1986	Joyce	5,300,926 A	4/1994	Stoeckl
4,616,637 A	10/1986	Caspari et al.	5,303,148 A	4/1994	Mattson et al.
4,624,011 A	11/1986	Watanabe et al.	5,304,185 A	4/1994	Taylor
4,633,389 A	12/1986	Tanaka et al.	5,305,203 A	4/1994	Raab
4,635,292 A	1/1987	Mori et al.	5,305,427 A	4/1994	Nagata
4,641,292 A	2/1987	Tunnell et al.	5,309,717 A	5/1994	Minch
4,655,257 A	4/1987	Iwashita	5,313,306 A	5/1994	Kuban et al.
4,672,963 A	6/1987	Barken	5,320,630 A	6/1994	Ahmed
4,676,243 A	6/1987	Clayman	5,337,732 A	8/1994	Grundfest et al.
4,728,974 A	3/1988	Nio et al.	5,339,799 A	8/1994	Kami et al.
4,762,455 A	8/1988	Coughlan et al.	5,343,385 A	8/1994	Joskowicz et al.
4,791,934 A	12/1988	Brunnett	5,343,391 A	8/1994	Mushabac
4,791,940 A	12/1988	Hirschfeld et al.	5,345,538 A	9/1994	Narayannan et al.
4,794,912 A	1/1989	Lia	5,357,962 A	10/1994	Green
4,815,006 A	3/1989	Andersson et al.	5,368,015 A	11/1994	Wilk
4,815,450 A	3/1989	Patel	5,368,428 A	11/1994	Hussey et al.
4,837,734 A	6/1989	Ichikawa et al.	5,371,536 A	12/1994	Yamaguchi
4,852,083 A	7/1989	Niehaus et al.	5,382,885 A	1/1995	Salcudean et al.
4,853,874 A	8/1989	Iwamoto et al.	5,388,987 A	2/1995	Badoz et al.
4,854,301 A	8/1989	Nakajima	5,395,369 A	3/1995	McBrayer et al.
4,860,215 A	8/1989	Seraji	5,397,323 A	3/1995	Taylor et al.
4,863,133 A	9/1989	Bonnell	5,402,801 A	4/1995	Taylor
4,883,400 A	11/1989	Kuban et al.	5,403,319 A	4/1995	Matsen, III et al.
4,930,494 A	6/1990	Takehana et al.	5,408,409 A	4/1995	Glassman et al.
4,945,479 A	7/1990	Rusterholz et al.	5,410,638 A	4/1995	Colgate et al.
4,949,717 A	8/1990	Shaw	5,417,210 A	5/1995	Funda et al.
4,954,952 A	9/1990	Ubhayakar et al.	5,417,701 A	5/1995	Holmes
4,965,417 A	10/1990	Massie	5,422,521 A	6/1995	Neer et al.
4,969,709 A	11/1990	Sogawa et al.	5,431,645 A	7/1995	Smith et al.
4,969,890 A	11/1990	Sugita et al.	5,434,457 A	7/1995	Josephs et al.
4,979,933 A	12/1990	Runge	5,442,728 A	8/1995	Kaufman et al.
4,979,949 A	12/1990	Matsen, III et al.	5,445,166 A	8/1995	Taylor
4,980,626 A	12/1990	Hess et al.	5,451,924 A	9/1995	Massimino et al.
4,989,253 A	1/1991	Liang et al.	5,454,827 A	10/1995	Aust et al.
4,996,975 A	3/1991	Nakamura	5,455,766 A	10/1995	Scheller et al.
5,019,968 A	5/1991	Wang et al.	5,458,547 A	10/1995	Teraoka et al.
5,020,001 A	5/1991	Yamamoto et al.	5,458,574 A	10/1995	Machold et al.
5,053,687 A	10/1991	Merlet	5,474,571 A	12/1995	Lang
5,065,741 A	11/1991	Uchiyama et al.	5,476,010 A	12/1995	Fleming et al.
5,078,140 A	1/1992	Kwoh	5,478,351 A	12/1995	Meade et al.
5,086,401 A	2/1992	Glassman et al.	5,489,292 A	2/1996	Tovey et al.
5,091,656 A	2/1992	Gahn	5,490,117 A	2/1996	Oda et al.
5,097,829 A	3/1992	Quisenberry	5,506,912 A	4/1996	Nagasaki et al.
5,097,839 A	3/1992	Allen	5,512,919 A	4/1996	Araki
5,098,426 A	3/1992	Sklar et al.	5,515,478 A	5/1996	Wang
5,105,367 A	4/1992	Tsuchihashi et al.	5,544,654 A	8/1996	Murphy et al.
5,109,499 A	4/1992	Inagami et al.	5,553,198 A	9/1996	Wang et al.
5,123,095 A	6/1992	Papadopoulos et al.	5,562,503 A	10/1996	Ellman et al.
5,131,105 A	7/1992	Harrowood et al.	5,571,110 A	11/1996	Matsen, III et al.
5,142,930 A	9/1992	Allen et al.	5,572,999 A	11/1996	Funda et al.
5,145,227 A	9/1992	Monford, Jr.	5,609,560 A	3/1997	Ichikawa et al.
5,166,513 A	11/1992	Keenan et al.	5,626,595 A	5/1997	Sklar et al.
5,175,694 A	12/1992	Amato	5,629,594 A	5/1997	Jacobus et al.
5,182,641 A	1/1993	Diner et al.	5,630,431 A	5/1997	Taylor
5,184,601 A	2/1993	Putman	5,631,973 A	5/1997	Green
5,187,574 A	2/1993	Kosemura et al.	5,636,259 A	6/1997	Khutoryansky et al.
5,196,688 A	3/1993	Hesse et al.	5,649,956 A	7/1997	Jensen et al.
5,201,325 A	4/1993	McEwen et al.	5,657,429 A	8/1997	Wang et al.
5,201,743 A	4/1993	Haber et al.	5,658,250 A	8/1997	Blomquist et al.
5,217,003 A	6/1993	Wilk	5,676,673 A	10/1997	Ferre et al.
5,221,283 A	6/1993	Chang	5,693,071 A	12/1997	Gorecki et al.
5,228,429 A	7/1993	Hatano	5,695,500 A	12/1997	Taylor et al.
5,230,623 A	7/1993	Guthrie et al.	5,696,574 A	12/1997	Schwaegerle
5,236,432 A	8/1993	Matsen, III et al.	5,696,837 A	12/1997	Green
5,239,883 A	8/1993	Rosheim	5,715,729 A	2/1998	Toyama et al.
5,251,127 A	10/1993	Raab	5,718,038 A	2/1998	Takiar et al.
5,257,999 A	11/1993	Slanetz, Jr.	5,727,569 A	3/1998	Benetti et al.
			5,735,290 A	4/1998	Sterman et al.
			5,737,711 A	4/1998	Abe
			5,740,699 A	4/1998	Ballantyne et al.
			5,749,362 A	5/1998	Funda et al.



(56)

References Cited

U.S. PATENT DOCUMENTS

5,754,741	A	5/1998	Wang et al.	
5,762,458	A	6/1998	Wang et al.	
5,766,126	A	6/1998	Anderson	
5,776,126	A	7/1998	Wilk et al.	
5,779,623	A	7/1998	Bonnell	
5,792,135	A	8/1998	Madhani et al.	
5,792,178	A	8/1998	Welch et al.	
5,797,900	A	8/1998	Madhani et al.	
5,800,423	A	9/1998	Jensen	
5,807,284	A	9/1998	Foxlin	
5,807,377	A	9/1998	Madhani et al.	
5,807,378	A	9/1998	Jensen et al.	
5,808,665	A	9/1998	Green	
5,810,879	A	9/1998	De Guillebon	
5,810,880	A	9/1998	Jensen et al.	
5,813,813	A	9/1998	Daum et al.	
5,814,038	A	9/1998	Jensen et al.	
5,817,084	A	10/1998	Jensen	
5,825,982	A	10/1998	Wright et al.	
5,836,869	A	11/1998	Kudo et al.	
5,844,824	A	12/1998	Newman et al.	
5,855,583	A	1/1999	Wang et al.	
5,859,934	A	1/1999	Green	
5,860,995	A *	1/1999	Berkelaar	606/174
5,876,325	A	3/1999	Mizuno et al.	
5,878,193	A	3/1999	Wang et al.	
5,882,206	A	3/1999	Gillio	
5,887,121	A	3/1999	Funda et al.	
5,904,702	A	5/1999	Ek et al.	
5,906,630	A	5/1999	Anderhub et al.	
5,931,832	A	8/1999	Jensen	
5,938,678	A	8/1999	Zirps et al.	
5,950,629	A	9/1999	Taylor et al.	
5,951,475	A	9/1999	Guezic et al.	
5,951,587	A	9/1999	Qureshi et al.	
5,954,731	A	9/1999	Yoon	
5,980,782	A	11/1999	Hershkowitz et al.	
5,984,932	A	11/1999	Yoon	
6,024,695	A	2/2000	Taylor et al.	
6,102,850	A	8/2000	Wang et al.	
6,120,433	A	9/2000	Mizuno et al.	
6,132,441	A *	10/2000	Grace	606/147
6,196,081	B1	3/2001	Yau	
6,270,453	B1	8/2001	Sakai	
6,307,285	B1	10/2001	Delson et al.	
6,312,435	B1	11/2001	Wallace et al.	
6,330,837	B1	12/2001	Charles et al.	
6,436,107	B1	8/2002	Wang et al.	
6,699,235	B2	3/2004	Wallace et al.	
6,793,669	B2	9/2004	Nakamura et al.	
RE43,049	E	12/2011	Grace	
8,292,916	B2	10/2012	Grace	
2008/0103524	A1	5/2008	Grace	

FOREIGN PATENT DOCUMENTS

DE	4310842	1/1995
DE	29803734 U1	4/1998
EP	239409	9/1987
EP	424687	5/1991
EP	776738	6/1997
WO	9104711	4/1991
WO	9220295	11/1992
WO	9313916	7/1993
WO	9418881	9/1994
WO	9426167	11/1994
WO	9715240	5/1997
WO	9825666	6/1998
WO	9834543 A1	8/1998
WO	9858589 A1	12/1998

OTHER PUBLICATIONS

Vertut, Jean and Phillipe Coiffet, Robot Technology: Teleoperation and Robotics Evolution and Development, English translation,

Prentice-Hall, Inc., Inglewood Cliffs, NJ, USA 1986, vol. 3A, 332 pages.

Abstract of a presentation "3-D Vision Technology Applied to Advanced Minimally Invasive Surgery Systems," (Session 15/3) given at the 3rd World Congress of Endoscopic Surgery in Bordeaux, Jun. 18-20, 1992, 1 page.

Abstract of a presentation "A Pneumatic Controlled Sewing Device for Endoscopic Application the MIS Sewing Instrument MSI" given at the 3rd World Congress of Endoscopic Surgery in Bordeaux, Jun. 18-20, 1992, 1 page.

Abstract of a presentation given at the 3rd World Congress of Endoscopic Surgery in Bordeaux entitled "Session 15/1", Jun. 18-20, 1992, 1 page.

Abstract of a presentation given at the 3rd World Congress of Endoscopic Surgery in Bordeaux, entitled "Session 15/2", Jun. 18-20, 1992, 1 page total.

Abstract of a presentation given at the 3rd World Congress of Endoscopic Surgery in Bordeaux entitled "Session 15/4", Jun. 18-20, 1992, 1 page.

Abstract of a presentation given at the 3rd World Congress of Endoscopic Surgery in Bordeaux entitled "Session 15/5", Jun. 18-20, 1992, 1 page.

Bejczy, Antal K. et al., "Controlling Remote Manipulators through Kinesthetic Coupling," Computers in Mechanical Engineering, 1983, pp. 48-60, vol. 1—Issue 1.

Ben Gayed, M. et al., "An Advanced Control Micromanipulator for Surgical Applications," Systems Science, 1987, pp. 123-134, vol. 13.

Besant, Colin et al., Abstract of presentation "Camera Control for Laparoscopic Surgery by Speech recognizing Robot: Constant Attention and Better Use of Personnel," 3rd World Congress of Endoscopic surgery, 1993, p. 271, vol. 3—issue 3.

Charles, Steve et al., "Design of a Surgeon Machine Interface for Teleoperated Microsurgery," Proceedings of IEEE Annual Conference on Engineering in Medicine and Biology, 1989, pp. 0883-0884, vol. 11, IEEE.

Colgate, Edward, J., "Power and Impedance Scaling in Bilateral Manipulation," IEEE International Conference on Robotics and Automation, Sacramento, California, Apr. 1991, pp. 2292-2297, vol. 3, IEEE.

Corcoran, Elizabeth, "Robots for the Operating Room," The New York Times, 2 pages total, Jul. 19, 1992, Section 3 p. 9C.

Das, Hari et al., "Kinematic Control and Visual Display of Redundant Teleoperators," IEEE International Conference on Systems, Man, and Cybernetics, 1989, pp. 1072-1077, vol. 3, IEEE.

Dolan, J.M. et al., "A Robot in an Operating Room: A Bull in a China Shop," 1987, pp. 1096-1097, vol. 2.

Green, Philip S. et al., Abstract of a presentation, "Telepresence: Advanced Teleoperator Technology for Minimally Invasive Surgery," 1992 Medicine Meets Virtual Reality (MMVR) symposium in San Diego, Jun. 4-7, 1992, 1 page.

Green, Philip S. et al., Statutory Declaration by Dr. Phillip S. Green, the presenter of the video entitled "Telepresence Surgery: The Future of Minimally Invasive Medicine," European Patent Convention in the Matter of EP-B-653922. 32 pages, Sep. 12, 2000.

Guerrouad, Aicha et al., "SMOS: Stereotaxical Microtelemanipulator for Ocular Surgery," IEEE Engineering in Medicine & Biology Society 11th annual international conference, Nov. 9-12, 1989, pp. 879-880, vol. 3, IEEE.

Inoue, Masao; "Six-Axis bilateral control of an articulated slave manipulator using a Cartesian master manipulator," Advanced robotics, 1990, pp. 139-150, vol. 4—Issue 2, Robotic society of Japan.

Jau, B. M., "Anthropomorphic Remote Manipulator," NASA Tech Briefs, Apr. 1991, p. 92, NASA's Jet Propulsion Laboratory, Pasadena, California.

Kazerooni, H., "Human/Robot Interaction via the Transfer of Power and Information Signals Part I: Dynamics and Control Analysis," IEEE International Conference on Robotics and Automation, 1989, pp. 1632-1640, IEEE.

Kazerooni, H., "Human/Robot Interaction via the Transfer of Power and Information Signals—Part II," An Experimental Analysis, Proc. of the 1989 IEEE International Conference on Robotics and Automation, 1989, pp. 1641-1647, vol. 3, IEEE.

(56)

**References Cited**

## OTHER PUBLICATIONS

Krishnan, S.M. et al., Abstract of a presentation "Design Considerations of a New Generation Endoscope Using Robotics and Computer Vision Technology," given at the 3rd World Congress of Endoscopic Surgery in Bordeaux, Jun. 18-20, 1992, 1 page.

Lavallee, Stephane, "A New System for Computer Assisted Neurosurgery," IEEE Eng. in Med. & Biol. Soc. 11th Annual International Conference, Jun. 1989, pp. 926-927, vol. 11.

Mair, Gordon M., Industrial Robotics, Prentice Hall, 1988, pp. 41-43, 49-50, 54, 203-209.

Majima S. et al., "On a Micro Manipulator for Medical Application Stability Consideration of its Bilateral Controller Mechatronics," 1991, pp. 293-309, vol. 1—Issue 3.

Melzer, Abstract of a presentation "Concept and Experimental Application of a Surgical Robotic System the Steerable MIS Instrument SMI," given at the 3rd World Congress of Endoscopic Surgery in Bordeaux, Jun. 18-20, 1992, 1 page total.

Preising, B. et al., "A Literature Review: Robots in Medicine," IEEE Engineering in Medicine and Biology, 1991, pp. 13-22, 71, vol. 10—Issue 2, IEEE.

Sabatini, A. M. et al., "Force Feedback Based Telemicromanipulation for Robot Surgery on Soft Tissue," IEEE Engineering in Medicine and Biology Society 11th Annual International Conference, 1989, pp. 890-891, vol. 3, IEEE.

Taubes, Gary et al., "Surgery in Cyberspace," Discover magazine, Dec. 1994, vol. 15, issue 12, pp. 85-92.

Taylor, Russell H. et al., "Taming the Bull: Safety in a Precise Surgical Robot," Fifth International Conference on Advanced Robotics (91 ICAR), Jun. 19-22, 1991, vol. 1, pp. 865-870, IEEE.

Tejima, Noriyuki et al., "A New Microsurgical Robot System for Corneal Transplantation," Precision Machinery, 1988, pp. 1-9, vol. 2, Gordon and Breach Science Publishers Inc.

Tendick Frank, et al., "Analysis of the Surgeon's Grasp for Telerobotic Surgical Manipulation," IEEE 11th Annual Int Conf on Engineering in Medicine and Biology, Jun. 1989, pp. 914-915, IEEE.

Thring, M.W., Robots and Telechairs: Manipulators with Memory; Remote Manipulators; Machine Limbs for the Handicapped, 1983, pp. 9-11, 108-131, 194-195, 235-279; Ellis Horwood Limited, Chapter 5,7,8,9.

Transcript of a video presented by SRI at the 3rd World Congress of Endoscopic Surgery in Bordeaux, France on Jun. 18-20, 1992; in Washington D.C. on Apr. 9, 1992; and in San Diego, CA on Jun. 4-7, 1992; entitled "Telepresence Surgery: The Future of Minimally Invasive Medicine," 3 pages.

Trevelyan, James P. et al., "Motion Control for a Sheep Shearing Robot," IEEE Robotics Research Conference, the 1st International Symposium, Carroll, NH, USA., 1983, pp. 175-190, in Robotics Research, MIT Press.

Vibet, C., "Properties of Master Slave Robots," Motor-con, 1987, pp. 309-316.


Wolf, Stanley et al., Student Reference Manual for Electronic Instrumentation Laboratories, 1990, pp. 498 and 499, Prentice Hall New Jersey.

PCT/US00/09201 International Search Report, mailed Aug. 30, 2000, 1 page.

Supplementary European Search Report for Application No. EP00914788, mailed on Mar. 11, 2009, 5 pages.

\* cited by examiner



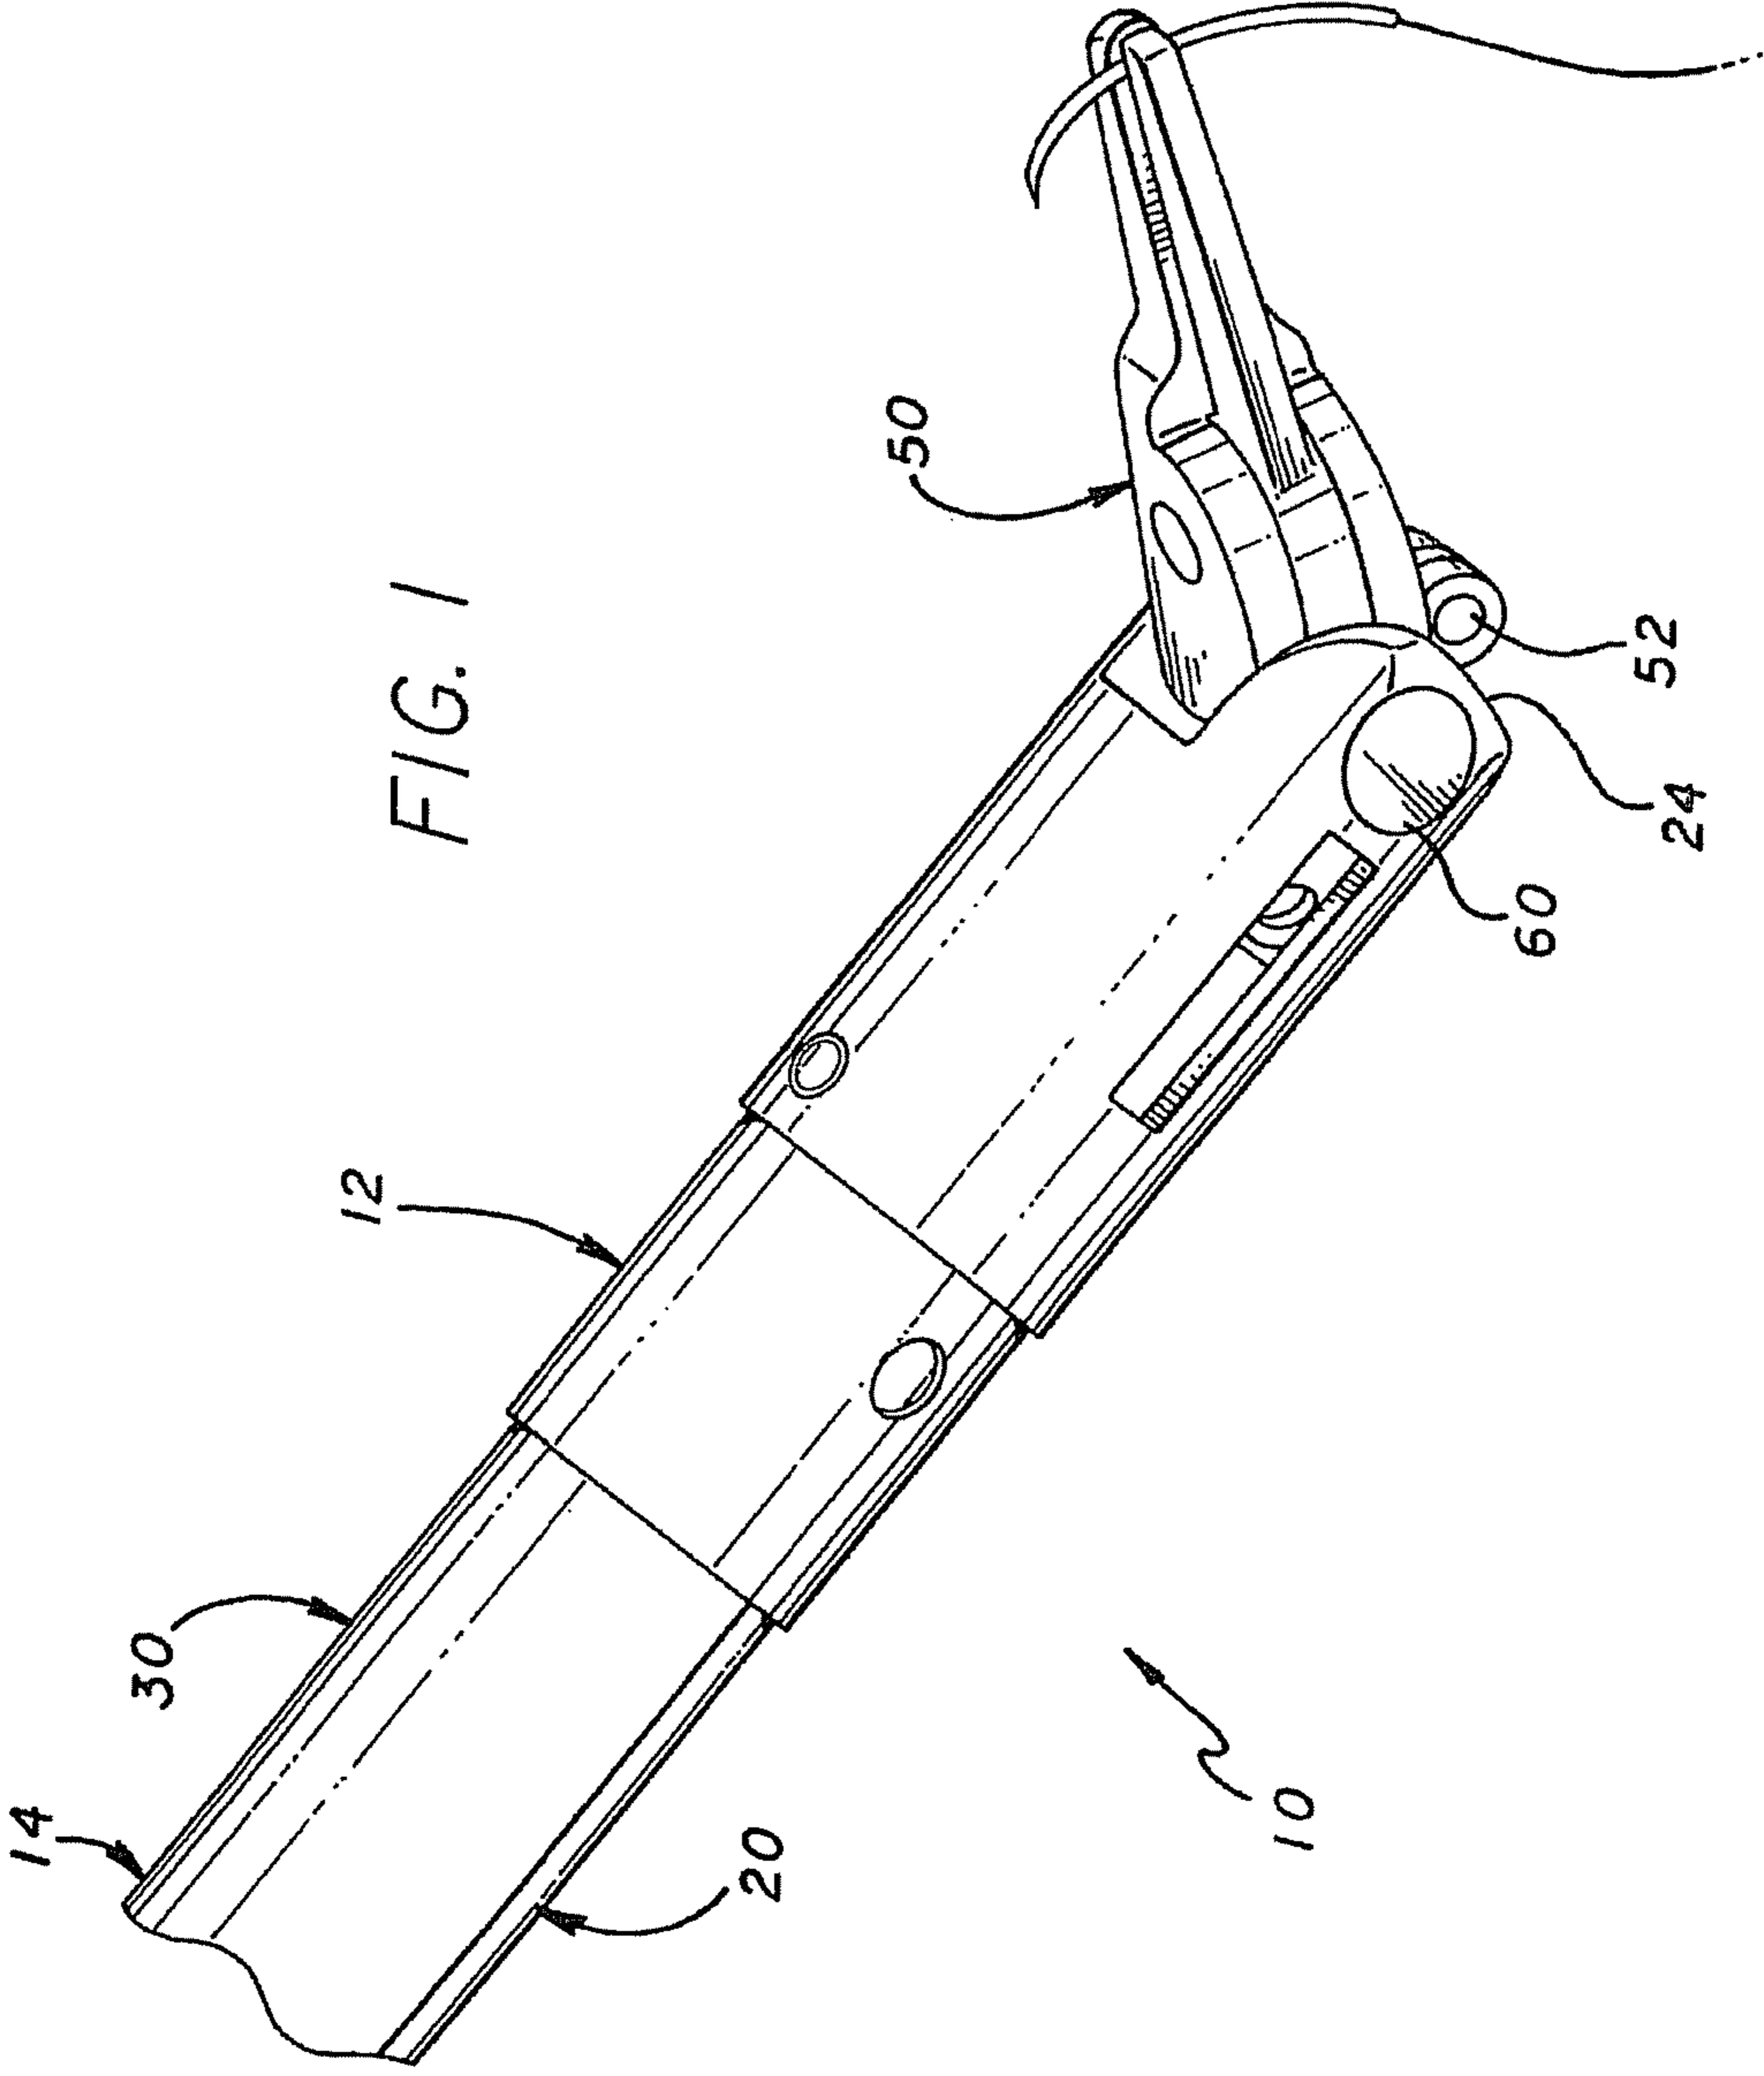


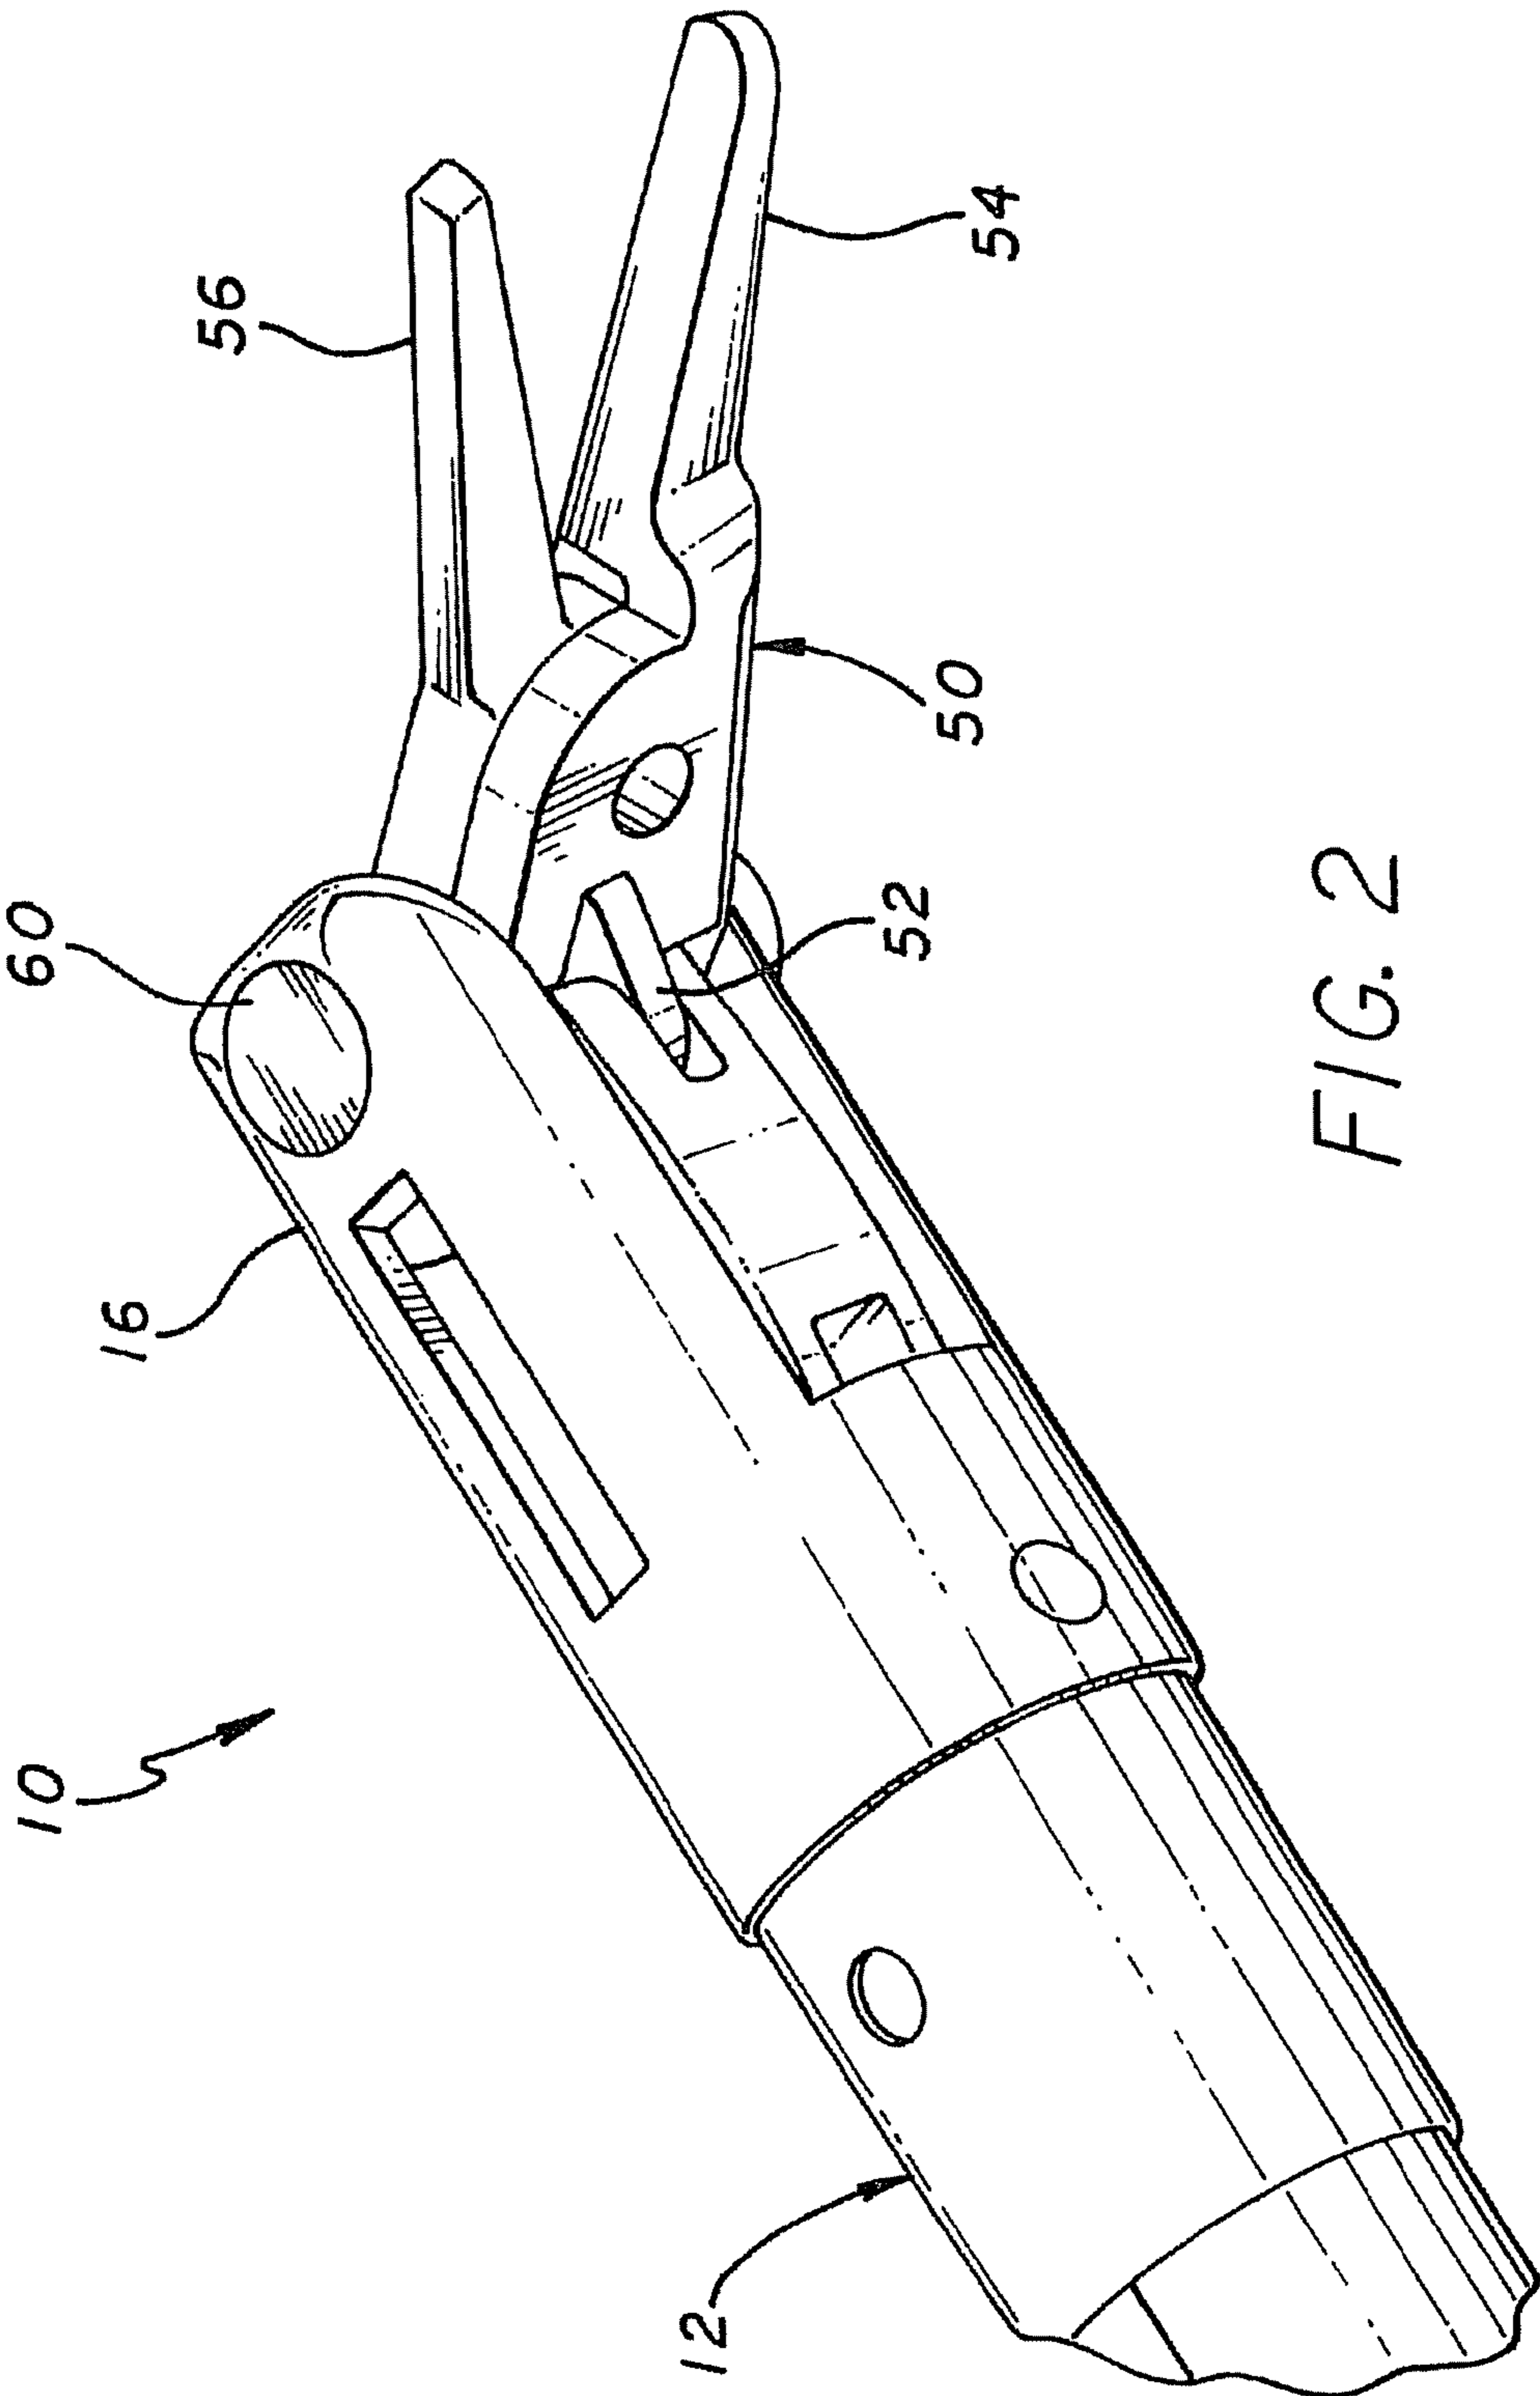


FIG. 2

FIG. 3



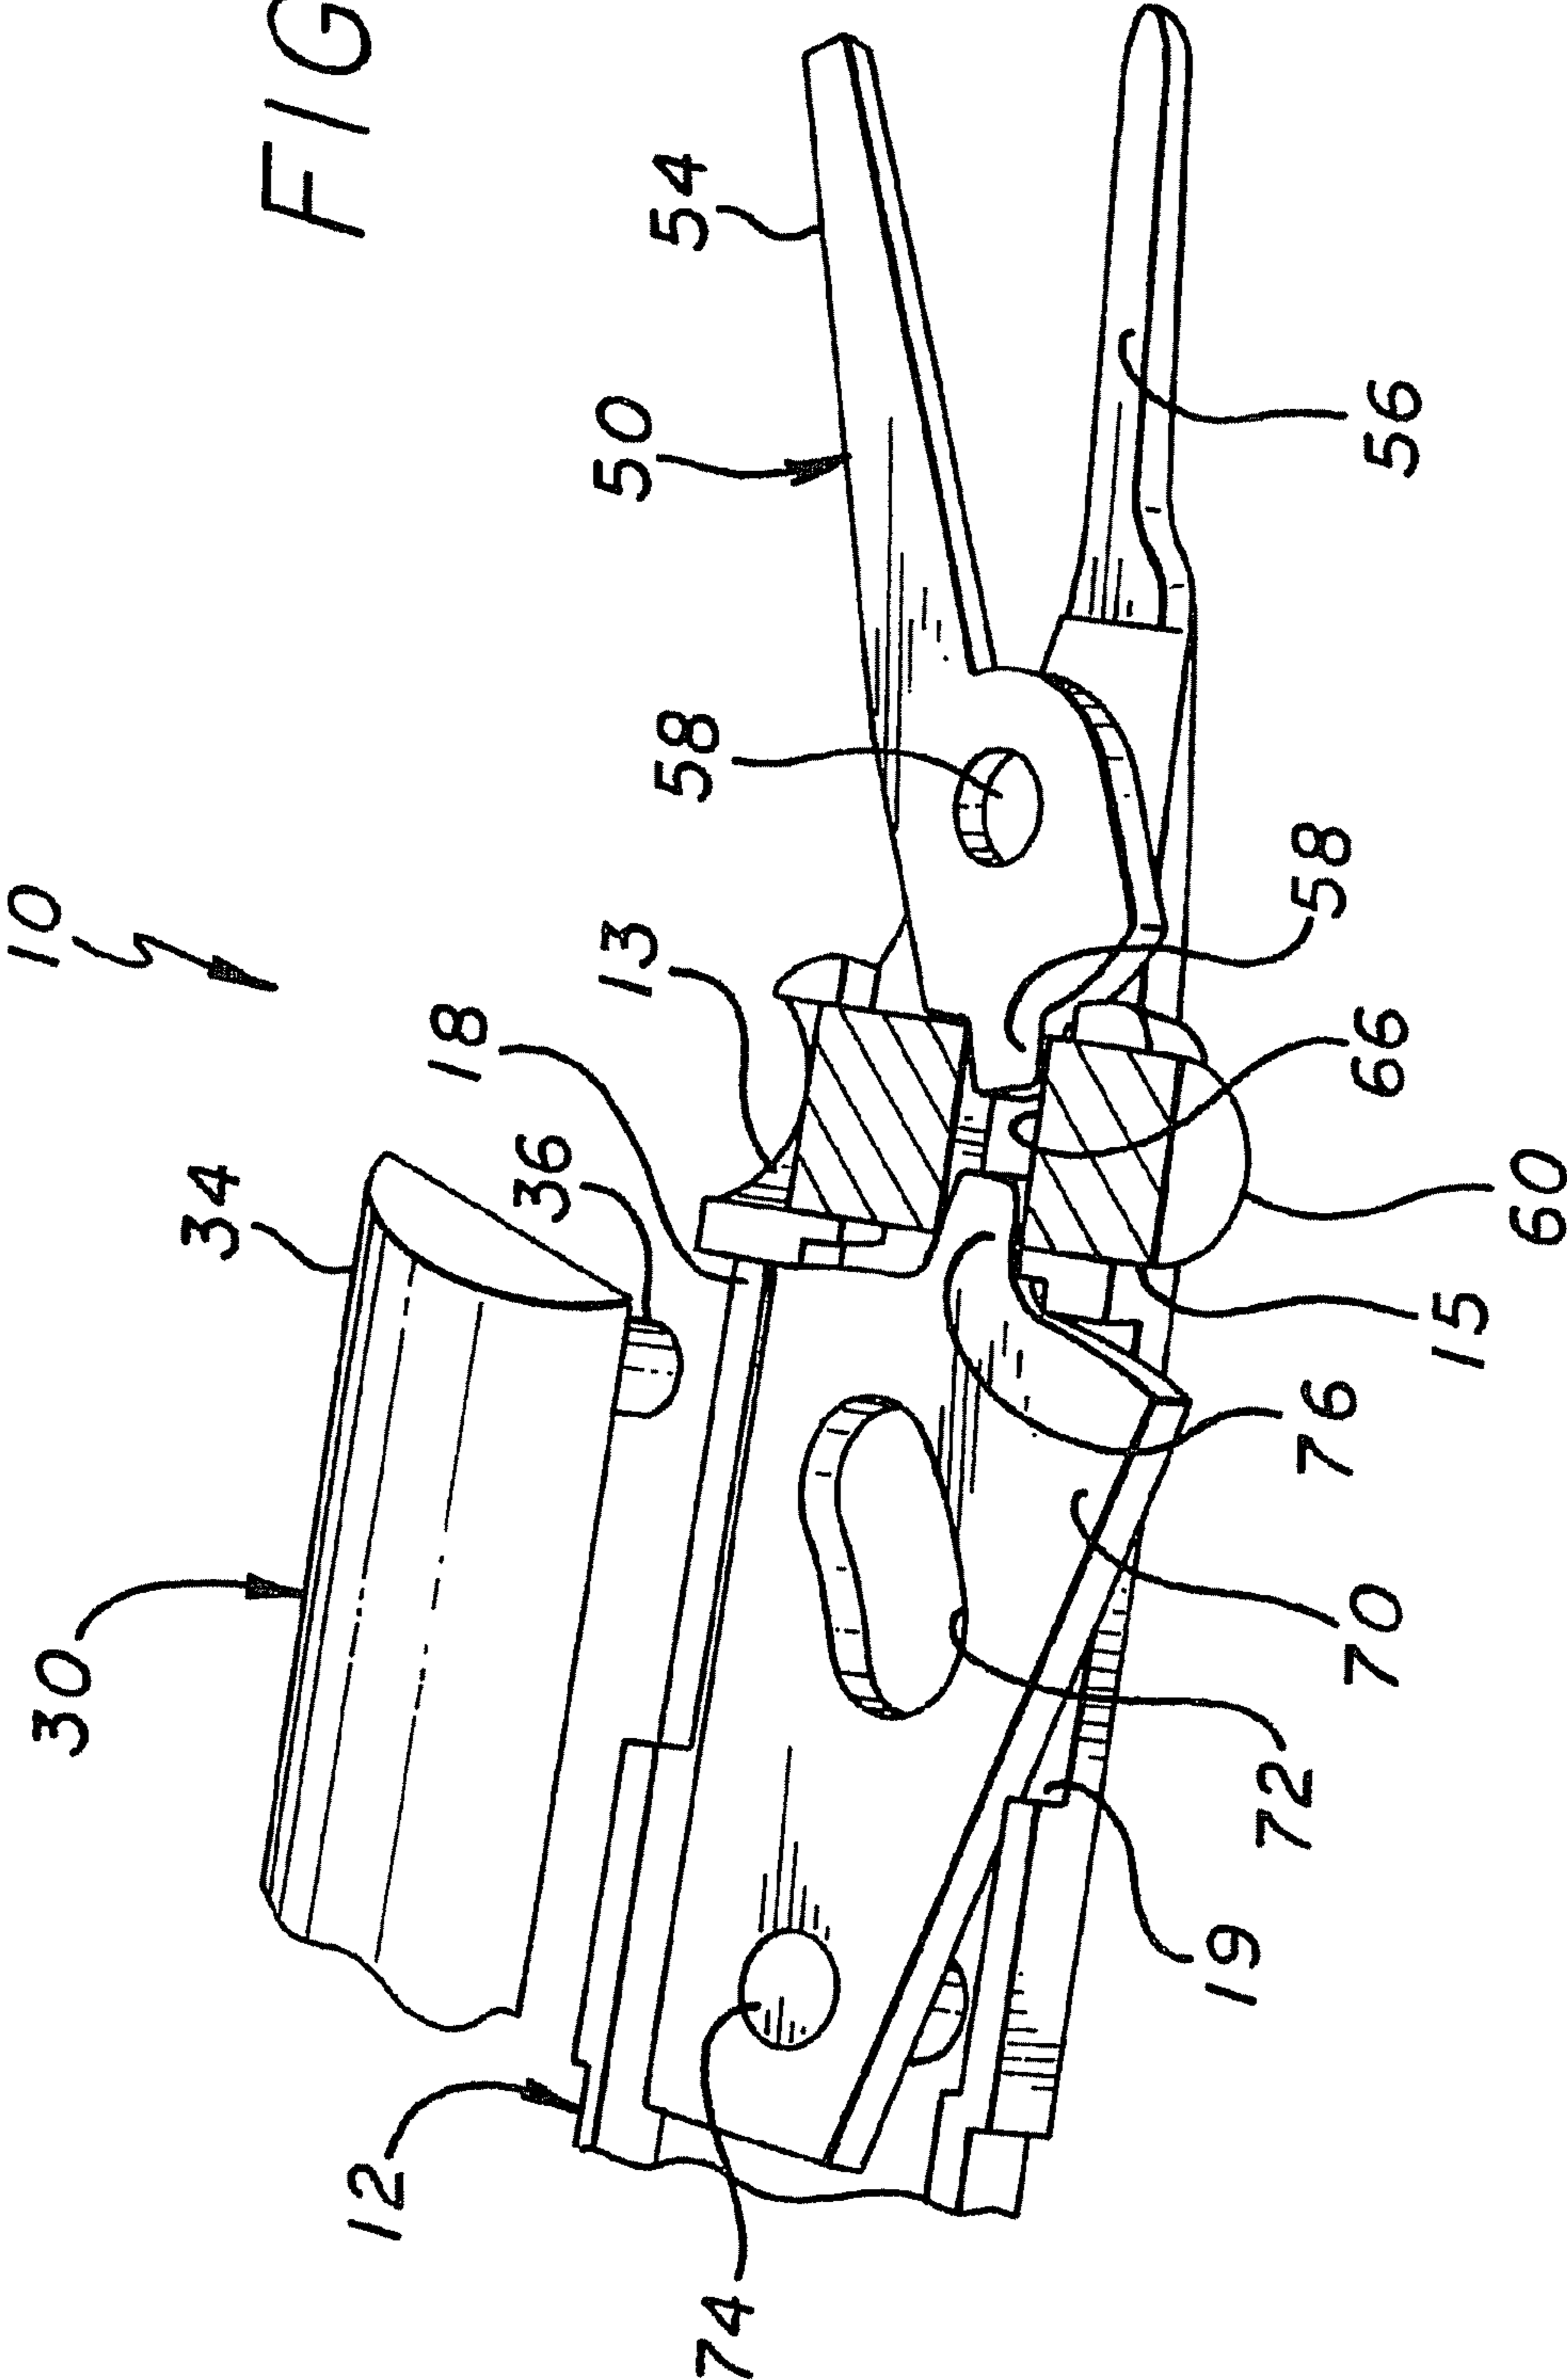

# RIGIDLY-LINKED ARTICULATING WRIST WITH DECOUPLED MOTION TRANSMISSION

## CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation-in-part of application Ser. No. 09/262,134, filed Mar. 3, 1999, which is a continuation-in-part of application Ser. No. 08/873,190, filed Jun. 11, 1997, now U.S. Pat. No. 6,102,850, which is a continuation-in-part of application Ser. No. 08/755,063, filed Nov. 22, 1996, now U.S. Pat. No. 5,855,583.

## BACKGROUND OF THE INVENTION

### 1. Field of the Invention

The present invention generally relates to surgical devices. More particularly, the present invention relates to a device for suturing during the performance of minimally invasive endoscopic surgical procedures and more particularly to an articulating device for use in endoscopic coronary artery by-pass grafting surgery.

### 2. Description of Related Art

Blockage of a coronary artery may deprive the heart of the blood and oxygen required to sustain life. The blockage may be removed with medication or by an angioplasty. For severe blockage, a coronary artery bypass graft (CABG) is performed to bypass the blocked area of the artery. CABG procedures are typically performed by splitting the sternum and pulling open the chest cavity to provide access to the heart. An incision may be made in the artery adjacent to the blocked area. The internal mammary artery (IMA) or some other arterial source of blood-flow may then be severed and attached to the artery at the point of incision. The IMA bypasses the blocked area of the artery to again provide a full flow of blood to the heart.

Splitting the sternum and opening the chest cavity can create tremendous trauma on the patient. Additionally, the cracked sternum prolongs the recovery period of the patient. As such, there have been developed systems that enable minimally invasive CABG procedures. These systems utilize hand held tools and small incisions, on the order of 3-5 inches in length, to provide access to the thoracic region of a patient.

Such minimally invasive procedures are conducted by inserting surgical instruments through small incisions, on the order of inches in the skin of the patient. Manipulating such instruments can be awkward, particularly when suturing a graft to an artery. These systems utilize direct visualization of the surgical site. Such systems do not enable a completely endoscopic approach to the CABG procedure because of the need for direct visualization of the site. Additionally, such systems do not enable a fully endoscopic approach because of the incision size necessary to adequately manipulate the surgical instruments at the surgical site.

A fully endoscopic approach utilizes small holes to provide access to the thoracic cavity. Each of these holes is on the order of 3-11 mm in diameter. In order to perform a CABG procedure in a fully endoscopic fashion (i.e. using 3-11 mm holes) a robotic system must be used to filter hand tremors and scale motions made by the surgeon.

To facilitate the performance of an endoscopic surgical procedure, it would be useful to employ surgical instruments that can maneuver to the surgical site as well as manipulate tissue or sutures to perform an anastomosis.

To help minimize risk to the patient, and to minimize operating time, what is needed in the art is a robotically

actuated surgical device that can articulate as well as actuate without being overly complex in design.

## SUMMARY OF THE INVENTION

The present invention is an articulating device for tissue and needle manipulation, the device comprising:

An elongated housing having a proximal end and a distal end;

an articulation rod extending interior the housing, the articulation rod having a proximal end and a distal end;

an actuation rod extending interior the housing, the actuation rod having a proximal end and a distal end;

a rack driver in communication with the actuation rod at the distal end thereof, the rack driver engaged with a cylindrical rack for translating the motion of the actuation rod substantially about ninety degrees; and

a jaw in communication with the cylindrical rack, whereby movement of the cylindrical rack actuates the jaw, the jaw further in pivotal communication with the articulation rod such that linear movement of the articulation rod produces rotational movement of the jaw.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a partial break-away perspective view of a device in accordance with the present invention in a closed angled configuration;

FIG. 2 is a partial break-away perspective view of a device in accordance with the present invention in an open angled configuration;

FIG. 3 is a cross-sectional perspective view of a device in accordance with the present invention in an opened straight configuration;

## DETAILED DESCRIPTION OF THE INVENTION

Referring to the drawings more particularly by reference numbers, FIGS. 1, 2 and 3 show a preferred embodiment of the articulating actuating device 10. The device 10 includes a housing 12. The housing extends substantially the length of the instrument 10 and has a proximal end 14 and a distal end 16 and a longitudinal axis X. Disposed interiorly the housing 12 is an articulation rod 20 and an actuation rod 30. Each of the articulation rod 20 and the actuation rod 30 have respective proximal ends 22, 32 and distal ends 24, 34.

The proximal ends 22, 32 of the rods may be attached to a robotic system for the performance of minimally invasive surgical procedures. One such system is produced by Computer Motion, Inc. The assignee hereof and is described in U.S. Pat. No. 5,855,583, which is incorporated herein by reference.

The rods 20, 30 are attached to actuators via attachment means taught in U.S. Pat. No. 5,855,583. Other means for removably attaching a rod to an actuator are known in the art including the use of screws, clips or the like. In this way, each of the rods 20, 30 may be driven by the actuator which is connected to various user interfaces and power sources and are conducive to the performance of minimally invasive surgical procedures.

The articulation rod 20 extends substantially the length of the housing 12 along its longitudinal axis X. The articulation rod 20 is pivotally connected to a jaw 50. Such a pivotal connection may be accomplished through the use of a hinge 52 attached intermediate the articulation rod 20 and the jaw 50.



The jaw **50** pivotally communicates with the housing **12** at the distal end **16** thereof through the use of a rack **60**. In this way, motion of the articulation rod **20** results in rotation of the jaw **50**. The rack **60** provides a pivot about which the jaw **50** rotates.

The actuation rod **30** provides for actuation of the jaw **50**. The actuation rod has a pin **36** disposed at the distal end **34** thereof. The pin **36** seats in a rack channel **72** disposed in a rack driver **70**. The rack driver is pivotally attached to the housing **12** via a pin **74** or the like. The housing has two longitudinal apertures **18, 19** formed therethrough at the distal end **16** thereof to provide for lateral movement of the rack driver **70** which shall be described in detail hereinbelow.

Longitudinal motion of the actuation rod **30** moves the pin **36** in the rack channel **72** which translates the longitudinal motion of the actuation rod **30** into a pivotal motion of the rack driver **70**. The rack driver **70** pivots about the pivot point defined by the pin **74** which attaches the rack driver **70** to the housing **12**. The rack driver **70** may move outside of the space defined as the interior of the housing through the longitudinal apertures **18, 19**.

The rack driver **70** has a shoulder **76** which engages the rack **60**. As the rack driver **70** pivots, the shoulder **76** causes the rack **60** to move laterally, which is orthogonal to the longitudinal motion of the actuation rod **30** and orthogonal to the longitudinal axis of the housing **12**. The rack **60** is slidably moveable within the housing **12** through two cylindrical apertures **13, 15** formed therethrough. As the rack **60** moves laterally, the jaw **50** is actuated. The lateral movement of the rack **60** is transferred to a first jaw element **54**. A second jaw element **56** is pivotally connected to the first jaw element **54** via a pin **58** or the like and is held stationary with respect to the first jaw element **54**. In this way, as the first jaw element is **54** is moved, the second jaw element **56** remains stationary and the jaw **50** is actuated. If each element has a sharp edge, then the jaw may function as a scissors.

The jaw **50** is always in communication with the rack **60**, even as it is articulated through the motion of the articulation rod **20**. This is accomplished through the use of a cylindrical rack having a circumferential channel **66** formed therein. The channel **66** receives the shoulder **76** of the rack driver **70** as well as a shoulder **58** on the first jaw element **54**. As such, as the jaw **50** is articulated, the shoulder **58** on the first jaw element **54** rotates within the circumferential channel **66** in the rack **60** maintaining communication therein and providing for actuation of the jaw **50** regardless of the articulated position of the jaw **50** caused through motion of the articulation rod **20**.

In this fashion, the articulation of the jaw **50** and the actuation of the jaw **50** are decoupled. It is highly advantageous to provide for a rigidly linked device that is decoupled in this fashion for several reasons. First, the device is easily sterilizable and secondly, the device is quite safe to use as there is no use of tensioned cables or the like.

While certain exemplary embodiments have been described and shown in the accompanying drawings, it is to be understood that such embodiments are merely illustrative of and not restrictive on the broad invention, and that this invention not be limited to the specific constructions and arrangements shown and described, since various other modifications may occur to those ordinarily skilled in the art.

What is claimed is:

1. A surgical instrument comprising:
  - a housing having a longitudinal axis, a proximal end, and a distal end;
  - a jaw element;
  - coupled to rotate the jaw element about a rotation axis;
  - an actuation rod having a distal end coupled to actuate the jaw element about an actuation axis, the actuation axis being orthogonal to the rotation axis;
  - a hinge attached intermediate the articulation rod and the jaw element; and
  - a rack coupled to the jaw element, the rack further being coupled to the articulation rod, the rack configured to rotate in response to the articulation rod being driven, the rack being a cylindrical rack having a circumferential channel formed therein.
2. The instrument of claim **1**, the actuation rod comprising a pin disposed at a distal end of the actuation rod, the instrument further comprising:
  - a rack driver pivotally attached to the housing, the rack driver comprising a rack channel fittingly receiving the pin of the actuation rod, the rack driver further having a distal end coupled to actuate the jaw element; wherein the rack driver comprises a shoulder engaging the rack.
3. The instrument of claim **1**, wherein at least one of the actuation rod and the articulation rod is removably attached to a corresponding actuator.
4. The instrument of claim **1**, further comprising a second jaw element, wherein the second jaw element is held stationary with respect to the jaw element.
5. The instrument of claim **1**, the articulation rod and the actuation rod being provided interior to the housing.
6. A surgical instrument comprising:
  - a housing having a longitudinal axis, a proximal end, and a distal end;
  - a jaw element;
  - coupled to rotate the jaw element about a rotation axis;
  - an actuation rod having a distal end coupled to actuate the jaw element about an actuation axis, the actuation axis being orthogonal to the rotation axis;
  - the actuation rod comprising a pin disposed at a distal end of the actuation rod, the instrument further comprising:
    - a rack driver pivotally attached to the housing, the rack driver comprising a rack channel fittingly receiving the pin of the actuation rod, the rack driver further having a distal end coupled to actuate the jaw element.
7. A surgical instrument comprising:
  - a housing having a longitudinal axis, a proximal end, and a distal end;
  - a jaw element;
  - an articulation rod having a distal end coupled to rotate the jaw element about a rotation axis;
  - an actuation rod having a distal end coupled to actuate the jaw element about an actuation axis, the actuation axis being orthogonal to the rotation axis;
  - a hinge attached intermediate the articulation rod and the jaw element; and
  - a rack coupled to the jaw element, the rack further being coupled to the articulation rod, the rack configured to rotate in response to the articulation rod being driven;
  - the housing comprising longitudinal apertures at the distal end thereof.

\* \* \* \* \*