



US009060689B2

(12) **United States Patent**
Tearney et al.

(10) **Patent No.:** **US 9,060,689 B2**
(45) **Date of Patent:** **Jun. 23, 2015**

(54) **APPARATUS, METHOD AND SYSTEM FOR PERFORMING PHASE-RESOLVED OPTICAL FREQUENCY DOMAIN IMAGING**

USPC 356/450-521
See application file for complete search history.

(75) Inventors: **Guillermo J. Tearney**, Cambridge, MA (US); **Brett Eugene Bouma**, Quincy, MA (US); **Johannes F. De Boer**, Somerville, MA (US); **Benjamin J. Vakoc**, Cambridge, MA (US); **Seok-Hyun Yun**, Cambridge, MA (US)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,339,754 A 1/1944 Brace
3,090,753 A 5/1963 Matuszak et al.

(Continued)

FOREIGN PATENT DOCUMENTS

CN 1550203 12/2004
DE 4309056 9/1994

(Continued)

OTHER PUBLICATIONS

Fujimoto et al., "High Resolution in Vivo Intra-Arterial Imaging with Optical Coherence Tomography," *Official Journal of the British Cardiac Society*, vol. 82, pp. 128-133 Heart, 1999.

(Continued)

Primary Examiner — Tarifur Chowdhury
Assistant Examiner — Michael P Lapage
(74) *Attorney, Agent, or Firm* — Andrews Kurth LLP

(73) Assignee: **The General Hospital Corporation**, Boston, MA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **11/445,990**

(22) Filed: **Jun. 1, 2006**

(65) **Prior Publication Data**

US 2006/0279742 A1 Dec. 14, 2006

Related U.S. Application Data

(60) Provisional application No. 60/686,790, filed on Jun. 1, 2005.

(51) **Int. Cl.**
G01N 21/55 (2014.01)
A61B 5/00 (2006.01)

(Continued)



(52) **U.S. Cl.**
CPC **A61B 5/0073** (2013.01); **G01B 9/02091** (2013.01); **A61B 5/0066** (2013.01); **A61B 2560/0223** (2013.01); **G01N 21/45** (2013.01); **G01N 21/4795** (2013.01); **G01N 21/49** (2013.01)

(58) **Field of Classification Search**
CPC A61B 5/0073; A61B 5/0066; A61B 2560/0223; G01N 21/49; G01N 21/4795; G01N 21/45; G01B 9/02091

(57) **ABSTRACT**

Apparatus, system and method are provided which utilize signals received from a reference and a sample. In particular, a radiation is provided which includes at least one first electro-magnetic radiation directed to the sample and at least one second electro-magnetic radiation directed to the reference. A frequency of the radiation varies over time. An interference can be detected between at least one third radiation associated with the first radiation and at least one fourth radiation associated with the second radiation. It is possible to obtain a particular signal associated with at least one phase of at least one frequency component of the interference, and compare the particular signal to at least one particular information. Further, it is possible to receive at least one portion of the radiation and provide a further radiation, such that the particular signal can be calibrated based on the further signal.

35 Claims, 15 Drawing Sheets

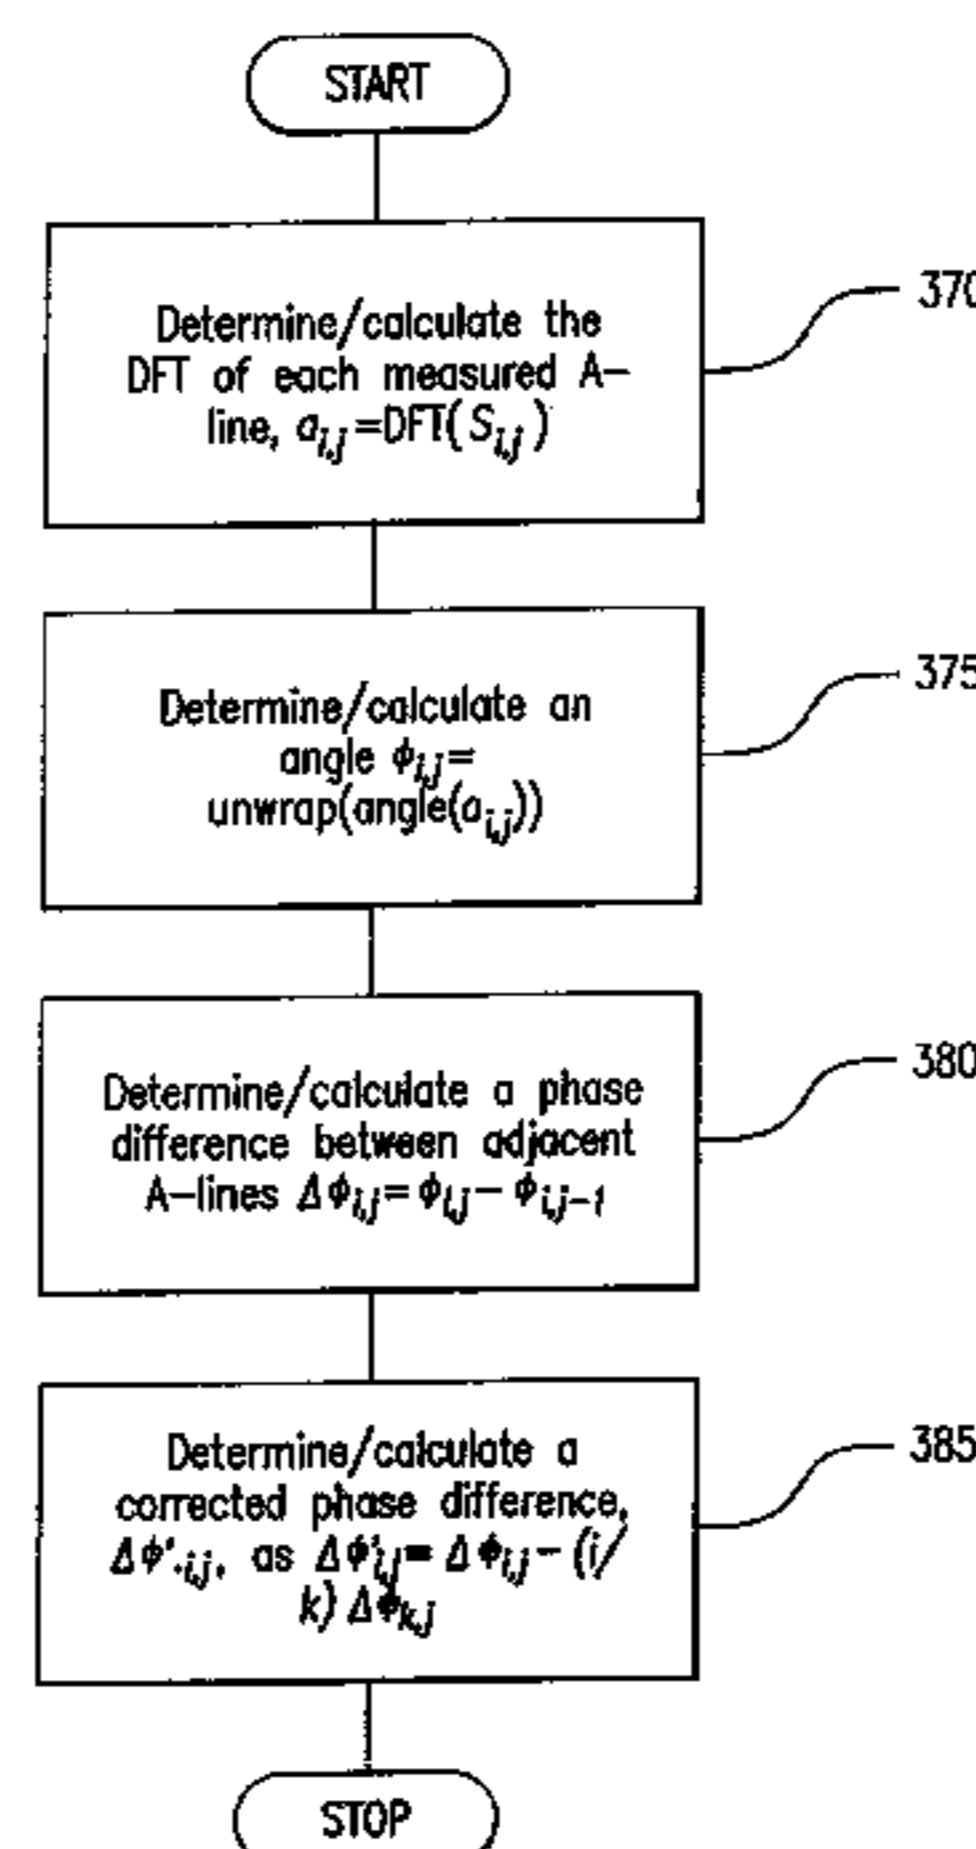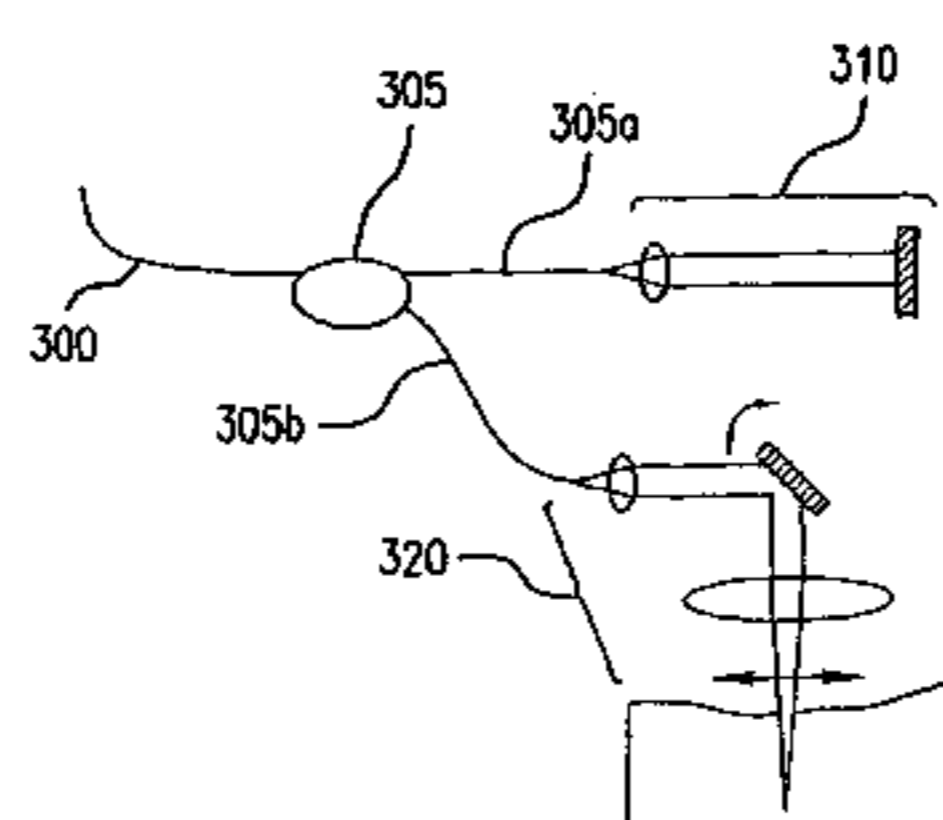

(51)	Int. Cl.		5,383,467 A	1/1995	Auer et al.
	<i>G01N 21/45</i>	(2006.01)	5,394,235 A	2/1995	Takeuchi et al.
	<i>G01N 21/47</i>	(2006.01)	5,400,771 A	3/1995	Pirak et al.
	<i>G01N 21/49</i>	(2006.01)	5,404,415 A	4/1995	Mori et al.
	<i>G01B 9/02</i>	(2006.01)	5,414,509 A	5/1995	Veligdan
			5,419,323 A	5/1995	Kittrell et al.
			5,424,827 A	6/1995	Horwitz et al.
			5,439,000 A	8/1995	Gunderson et al.
(56)	References Cited		5,441,053 A	8/1995	Lodder et al.
	U.S. PATENT DOCUMENTS		5,450,203 A	9/1995	Penkethman
			5,459,325 A	10/1995	Hueton et al.
			5,459,570 A	10/1995	Swanson et al.
			5,465,147 A	11/1995	Swanson
			5,486,701 A	1/1996	Norton et al.
			5,491,524 A	2/1996	Hellmuth et al.
			5,491,552 A	2/1996	Knuttel
			5,522,004 A	5/1996	Djupsjobacka et al.
			5,526,338 A	6/1996	Hasman et al.
			5,555,087 A	9/1996	Miyagawa et al.
			5,562,100 A	10/1996	Kittrell et al.
			5,565,983 A	10/1996	Barnard et al.
			5,565,986 A	10/1996	Knuttel
			5,566,267 A	10/1996	Neuberger
			5,583,342 A	12/1996	Ichie
			5,590,660 A	1/1997	MacAulay et al.
			5,600,486 A	2/1997	Gal et al.
			5,601,087 A	2/1997	Gunderson et al.
			5,623,336 A	4/1997	Raab et al.
			5,635,830 A	6/1997	Itoh
			5,649,924 A	7/1997	Everett et al.
			5,697,373 A	12/1997	Richards-Kortum et al.
			5,698,397 A	12/1997	Zarling et al.
			5,701,155 A	12/1997	Wood et al.
			5,710,630 A	1/1998	Essenpreis et al.
			5,719,399 A	2/1998	Alfano et al.
			5,730,731 A	3/1998	Mollenauer et al.
			5,735,276 A	4/1998	Lemelson
			5,748,318 A	5/1998	Maris et al.
			5,748,598 A	5/1998	Swanson et al.
			5,752,518 A	5/1998	McGee et al.
			5,784,352 A	7/1998	Swanson et al.
			5,785,651 A	7/1998	Kuhn et al.
			5,795,295 A	8/1998	Hellmuth et al.
			5,801,831 A	9/1998	Sargoytchev et al.
			5,803,082 A	9/1998	Stapleton et al.
			5,807,261 A	9/1998	Benaron et al.
			5,810,719 A	9/1998	Toida
			5,817,144 A	10/1998	Gregory et al.
			5,836,877 A	11/1998	Zavislan et al.
			5,840,023 A	11/1998	Oraevsky et al.
			5,840,031 A	11/1998	Crowley
			5,842,995 A	12/1998	Mahadevan-Jansen et al.
			5,843,000 A	12/1998	Nishioka et al.
			5,847,827 A	12/1998	Fercher
			5,865,754 A	2/1999	Sevick-Muraca et al.
			5,871,449 A	2/1999	Brown
			5,877,856 A	3/1999	Fercher
			5,887,009 A	3/1999	Mandella et al.
			5,910,839 A	6/1999	Erskine et al.
			5,912,764 A	6/1999	Togino
			5,920,373 A	7/1999	Bille
			5,920,390 A	7/1999	Farahi et al.
			5,921,926 A	7/1999	Rolland et al.
			5,926,592 A	7/1999	Harris et al.
			5,949,929 A	9/1999	Hamm
			5,951,482 A	9/1999	Winston et al.
			5,955,737 A	9/1999	Hallidy et al.
			5,956,355 A *	9/1999	Swanson et al. 372/20
			5,968,064 A	10/1999	Selmon et al.
			5,975,697 A	11/1999	Podoleanu et al.
			5,975,699 A	11/1999	Hellmuth et al.
			5,983,125 A	11/1999	Alfano et al.
			5,987,346 A	11/1999	Benaron et al.
			5,991,697 A	11/1999	Nelson et al.
			5,994,690 A *	11/1999	Kulkarni et al. 250/216
			5,995,223 A	11/1999	Power
			6,002,480 A	12/1999	Izatt et al.
			6,004,314 A	12/1999	Wei et al.
			6,006,128 A	12/1999	Izatt et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,007,996 A	12/1999	McNamara et al.	6,560,259 B1	5/2003	Hwang et al.
6,010,449 A	1/2000	Selmon et al.	6,564,087 B1	5/2003	Pitris et al.
6,016,197 A	1/2000	Krivoshlykov	6,564,089 B2	5/2003	Izatt et al.
6,020,963 A	2/2000	Dimarzio et al.	6,567,585 B2	5/2003	Harris
6,025,956 A	2/2000	Nagano et al.	6,593,101 B2	7/2003	Richards-Kortum et al.
6,033,721 A	3/2000	Nassuphis	6,611,833 B1	8/2003	Johnson et al.
6,037,579 A	3/2000	Chan et al.	6,622,732 B2	9/2003	Constantz
6,044,288 A	3/2000	Wake et al.	6,654,127 B2	11/2003	Everett et al.
6,045,511 A	4/2000	Ott et al.	6,657,730 B2	12/2003	Pfau et al.
6,048,742 A	4/2000	Weyburne et al.	6,658,278 B2	12/2003	Gruhl
6,052,186 A	4/2000	Tsai	6,680,780 B1	1/2004	Fee
6,053,613 A	4/2000	Wei et al.	6,685,885 B2	2/2004	Nolte et al.
6,069,698 A	5/2000	Ozawa et al.	6,687,007 B1	2/2004	Meigs
6,078,047 A	6/2000	Mittleman et al.	6,687,010 B1	2/2004	Horii et al.
6,091,984 A	7/2000	Perelman et al.	6,692,430 B2	2/2004	Adler
6,094,274 A	7/2000	Yokoi	6,701,181 B2	3/2004	Tang et al.
6,107,048 A	8/2000	Goldenring et al.	6,721,094 B1	4/2004	Sinclair et al.
6,111,645 A	8/2000	Tearney et al.	6,725,073 B1	4/2004	Motamedi et al.
6,117,128 A	9/2000	Gregory	6,738,144 B1	5/2004	Dogariu et al.
6,120,516 A	9/2000	Selmon et al.	6,741,884 B1	5/2004	Freeman et al.
6,134,003 A	10/2000	Tearney et al.	6,757,467 B1	6/2004	Rogers
6,134,010 A	10/2000	Zavitslan	6,790,175 B1	9/2004	Furusawa et al.
6,141,577 A	10/2000	Rolland et al.	6,806,963 B1	10/2004	Wälti et al.
6,151,522 A	11/2000	Alfano et al.	6,816,743 B2	11/2004	Moreno et al.
6,159,445 A	12/2000	Klaveness et al.	6,831,781 B2	12/2004	Tearney et al.
6,160,826 A	12/2000	Swanson et al.	6,839,496 B1	1/2005	Mills et al.
6,161,031 A	12/2000	Hochman et al.	6,882,432 B2	4/2005	Deck
6,166,373 A	12/2000	Mao	6,900,899 B2	5/2005	Nevis
6,175,669 B1	1/2001	Colston et al.	6,909,105 B1	6/2005	Heintzmann et al.
6,185,271 B1	2/2001	Kinsinger	6,949,072 B2	9/2005	Furnish et al.
6,191,862 B1	2/2001	Swanson et al.	6,961,123 B1	11/2005	Wang et al.
6,193,676 B1	2/2001	Winston et al.	6,980,299 B1	12/2005	de Boer
6,198,956 B1	3/2001	Dunne	6,996,549 B2	2/2006	Zhang et al.
6,201,989 B1	3/2001	Whitehead et al.	7,006,232 B2	2/2006	Rollins et al.
6,208,415 B1	3/2001	De Boer et al.	7,019,838 B2	3/2006	Izatt et al.
6,208,887 B1	3/2001	Clarke	7,027,633 B2	4/2006	Foran et al.
6,245,026 B1	6/2001	Campbell et al.	7,061,622 B2	6/2006	Rollins et al.
6,249,381 B1	6/2001	Suganuma	7,072,047 B2	7/2006	Westphal et al.
6,249,630 B1	6/2001	Stock et al.	7,075,658 B2	7/2006	Izatt et al.
6,272,268 B1	8/2001	Miller et al.	7,113,288 B2	9/2006	Fercher
6,282,011 B1	8/2001	Tearney et al.	7,113,625 B2	9/2006	Watson et al.
6,297,018 B1	10/2001	French et al.	7,130,320 B2	10/2006	Tobiason et al.
6,301,048 B1	10/2001	Cao	7,139,598 B2	11/2006	Hull et al.
6,308,092 B1	10/2001	Hoyns	7,142,835 B2	11/2006	Paulus
6,324,419 B1	11/2001	Guzelsu et al.	7,148,970 B2	12/2006	De Boer
6,341,036 B1	1/2002	Tearney et al.	7,177,027 B2	2/2007	Hirasawa et al.
6,353,693 B1	3/2002	Kano et al.	7,190,464 B2	3/2007	Alphonse
6,374,128 B1	4/2002	Toida et al.	7,230,708 B2	6/2007	Lapotko et al.
6,377,349 B1	4/2002	Fercher	7,236,637 B2	6/2007	Sirohey et al.
6,384,915 B1	5/2002	Everett et al.	7,242,480 B2	7/2007	Alphonse
6,393,312 B1	5/2002	Hoyns	7,267,494 B2	9/2007	Deng et al.
6,394,964 B1	5/2002	Sievert, Jr. et al.	7,272,252 B2	9/2007	De La Torre-Bueno et al.
6,396,941 B1	5/2002	Bacus et al.	7,304,798 B2	12/2007	Izumi et al.
6,421,164 B2	7/2002	Tearney et al.	7,310,150 B2	12/2007	Guillermo et al.
6,437,867 B2	8/2002	Zeylikovich et al.	7,321,431 B2 *	1/2008	De Groot 356/497
6,441,892 B2	8/2002	Xiao et al.	7,330,270 B2	2/2008	O'Hara et al.
6,441,959 B1	8/2002	Yang et al.	7,336,366 B2	2/2008	Choma et al.
6,445,485 B1	9/2002	Frigo et al.	7,342,659 B2	3/2008	Horn et al.
6,445,939 B1	9/2002	Swanson et al.	7,355,716 B2	4/2008	De Boer et al.
6,445,944 B1	9/2002	Ostrovsky	7,355,721 B2	4/2008	Quadling et al.
6,463,313 B1	10/2002	Winston et al.	7,359,062 B2	4/2008	Chen et al.
6,469,846 B2	10/2002	Ebizuka et al.	7,365,858 B2	4/2008	Fang-Yen et al.
6,475,159 B1	11/2002	Casscells et al.	7,366,376 B2	4/2008	Shishkov et al.
6,475,210 B1	11/2002	Phelps et al.	7,382,809 B2	6/2008	Chong et al.
6,477,403 B1	11/2002	Eguchi et al.	7,391,520 B2	6/2008	Zhou et al.
6,485,413 B1	11/2002	Boppart et al.	7,458,683 B2	12/2008	Chernyak et al.
6,485,482 B1	11/2002	Belef	7,530,948 B2	5/2009	Seibel et al.
6,501,551 B1	12/2002	Tearney et al.	7,539,530 B2	5/2009	Caplan et al.
6,516,014 B1	2/2003	Sellin et al.	7,609,391 B2	10/2009	Betzig
6,517,532 B1	2/2003	Altshuler et al.	7,630,083 B2	12/2009	de Boer et al.
6,538,817 B1	3/2003	Farmer et al.	7,643,152 B2	1/2010	de Boer et al.
6,540,391 B2	4/2003	Lanzetta et al.	7,643,153 B2	1/2010	de Boer et al.
6,549,801 B1	4/2003	Chen et al.	7,646,905 B2	1/2010	Guittet et al.
6,552,796 B2	4/2003	Magnin et al.	7,649,160 B2	1/2010	Colomb et al.
6,558,324 B1	5/2003	Von Behren et al.	7,664,300 B2	2/2010	Lange et al.
			7,733,497 B2	6/2010	Yun et al.
			7,782,464 B2	8/2010	Mujat et al.
			7,799,558 B1	9/2010	Dultz
			7,805,034 B2	9/2010	Kato et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,911,621 B2	3/2011	Motaghiannezam et al.	2004/0263843 A1	12/2004	Knopp et al.
7,969,578 B2	6/2011	Yun et al.	2005/0004453 A1	1/2005	Tearney et al.
7,973,936 B2	7/2011	Dantus	2005/0018133 A1	1/2005	Huang et al.
2001/0020126 A1	9/2001	Swanson et al.	2005/0018200 A1	1/2005	Guillermo et al.
2001/0036002 A1	11/2001	Tearney et al.	2005/0018201 A1	1/2005	De Boer et al.
2001/0047137 A1	11/2001	Moreno et al.	2005/0035295 A1	2/2005	Bouma et al.
2001/0055462 A1	12/2001	Seibel	2005/0036150 A1	2/2005	Izatt et al.
2002/0016533 A1	2/2002	Marchitto et al.	2005/0046837 A1	3/2005	Izumi et al.
2002/0024015 A1	2/2002	Hoffmann et al.	2005/0057680 A1	3/2005	Agan
2002/0037252 A1	3/2002	Toida et al.	2005/0057756 A1	3/2005	Fang-Yen et al.
2002/0048025 A1	4/2002	Takaoka	2005/0059894 A1	3/2005	Zeng et al.
2002/0048026 A1	4/2002	Isshiki et al.	2005/0065421 A1	3/2005	Burckhardt et al.
2002/0052547 A1	5/2002	Toida	2005/0119567 A1	6/2005	Choi et al.
2002/0057431 A1	5/2002	Fateley et al.	2005/0128488 A1	6/2005	Yelin et al.
2002/0086347 A1	7/2002	Johnson et al.	2005/0165303 A1	7/2005	Kleen et al.
2002/0091322 A1	7/2002	Chaiken et al.	2005/0171438 A1	8/2005	Chen et al.
2002/0109851 A1	8/2002	Deck	2005/0190372 A1	9/2005	Dogariu et al.
2002/0113965 A1	8/2002	Roche et al.	2005/0197530 A1	9/2005	Wallace et al.
2002/0122182 A1	9/2002	Everett et al.	2005/0221270 A1	10/2005	Connelly et al.
2002/0122246 A1	9/2002	Tearney et al.	2005/0254059 A1	11/2005	Alphonse
2002/0140942 A1	10/2002	Fee et al.	2005/0254061 A1	11/2005	Alphonse et al.
2002/0158211 A1	10/2002	Gillispie	2006/0020172 A1	1/2006	Luerssen et al.
2002/0161357 A1	10/2002	Anderson et al.	2006/0033923 A1	2/2006	Hirasawa et al.
2002/0163622 A1	11/2002	Magnin et al.	2006/0039004 A1	2/2006	De Boer et al.
2002/0166946 A1	11/2002	Iizuka et al.	2006/0093276 A1	5/2006	Bouma et al.
2002/0168158 A1	11/2002	Furusawa et al.	2006/0103850 A1	5/2006	Alphonse et al.
2002/0183623 A1	12/2002	Tang et al.	2006/0106375 A1	5/2006	Werneth et al.
2002/0196446 A1	12/2002	Roth et al.	2006/0146339 A1	7/2006	Fujita et al.
2002/0198457 A1	12/2002	Tearney et al.	2006/0164639 A1	7/2006	Horn et al.
2003/0001071 A1	1/2003	Mandella et al.	2006/0167363 A1	7/2006	Bernstein et al.
2003/0013973 A1	1/2003	Georgakoudi et al.	2006/0171503 A1	8/2006	O'Hara et al.
2003/0023153 A1	1/2003	Izatt et al.	2006/0184048 A1	8/2006	Saadat et al.
2003/0025917 A1	2/2003	Suhami	2006/0189928 A1	8/2006	Camus et al.
2003/0026735 A1	2/2003	Nolte et al.	2006/0224053 A1	10/2006	Black et al.
2003/0028114 A1	2/2003	Casscells, III et al.	2006/0244973 A1*	11/2006	Yun et al. 356/511
2003/0030816 A1	2/2003	Eom et al.	2006/0279742 A1	12/2006	Tearney
2003/0043381 A1	3/2003	Fercher	2007/0002435 A1	1/2007	Ye et al.
2003/0053673 A1	3/2003	Dewaele et al.	2007/0019208 A1	1/2007	Toida et al.
2003/0067607 A1	4/2003	Wolleschensky et al.	2007/0024860 A1	2/2007	Tobiason et al.
2003/0082105 A1	5/2003	Fischman et al.	2007/0035743 A1	2/2007	Vakoc et al.
2003/0097048 A1	5/2003	Ryan et al.	2007/0038040 A1	2/2007	Cense et al.
2003/0108911 A1	6/2003	Klimant et al.	2007/0048818 A1	3/2007	Rosen et al.
2003/0120137 A1	6/2003	Pawluczyk et al.	2007/0070496 A1	3/2007	Gweon et al.
2003/0135101 A1	7/2003	Webler	2007/0076217 A1	4/2007	Baker et al.
2003/0137669 A1	7/2003	Rollins et al.	2007/0086013 A1	4/2007	De Lega et al.
2003/0165263 A1	9/2003	Hamer et al.	2007/0086017 A1	4/2007	Buckland et al.
2003/0174339 A1	9/2003	Feldchtein et al.	2007/0091317 A1	4/2007	Freischlad et al.
2003/0218756 A1	11/2003	Chen et al.	2007/0133002 A1	6/2007	Wax et al.
2003/0220749 A1	11/2003	Chen et al.	2007/0188855 A1	8/2007	Shishkov et al.
2003/0236443 A1	12/2003	Cespedes et al.	2007/0203404 A1	8/2007	Zysk et al.
2004/0002650 A1	1/2004	Mandrusov et al.	2007/0208225 A1	9/2007	Czaniera et al.
2004/0039252 A1	2/2004	Koch	2007/0223006 A1	9/2007	Tearney et al.
2004/0039298 A1	2/2004	Abreu	2007/0233056 A1	10/2007	Yun
2004/0054268 A1	3/2004	Esenaliev et al.	2007/0233396 A1	10/2007	Tearney et al.
2004/0072200 A1	4/2004	Rigler et al.	2007/0236700 A1	10/2007	Yun et al.
2004/0075841 A1	4/2004	Van Neste et al.	2007/0253901 A1	11/2007	Deng et al.
2004/0076940 A1	4/2004	Alexander et al.	2007/0258094 A1	11/2007	Izatt et al.
2004/0077949 A1	4/2004	Blofgett et al.	2007/0291277 A1	12/2007	Everett et al.
2004/0085540 A1	5/2004	Lapotko et al.	2008/0002197 A1	1/2008	Sun et al.
2004/0095464 A1	5/2004	Miyagi et al.	2008/0007734 A1	1/2008	Park et al.
2004/0110206 A1	6/2004	Wong et al.	2008/0021275 A1	1/2008	Tearney et al.
2004/0126048 A1	7/2004	Dave et al.	2008/0049220 A1	2/2008	Izzia et al.
2004/0126120 A1	7/2004	Cohen et al.	2008/0070323 A1	3/2008	Hess et al.
2004/0150830 A1	8/2004	Chan	2008/0094613 A1	4/2008	de Boer et al.
2004/0152989 A1	8/2004	Puttappa et al.	2008/0094637 A1	4/2008	de Boer et al.
2004/0165184 A1	8/2004	Mizuno	2008/0097225 A1	4/2008	Tearney et al.
2004/0166593 A1	8/2004	Nolte et al.	2008/0097709 A1	4/2008	de Boer et al.
2004/0189999 A1*	9/2004	De Groot et al. 356/497	2008/0100837 A1	5/2008	de Boer et al.
2004/0204651 A1	10/2004	Freeman et al.	2008/0139906 A1	6/2008	Bussek et al.
2004/0239938 A1	12/2004	Izatt et al.	2008/0152353 A1	6/2008	de Boer et al.
2004/0246490 A1	12/2004	Wang	2008/0154090 A1	6/2008	Hashimshony
2004/0246583 A1	12/2004	Mueller et al.	2008/0192236 A1	8/2008	Smith et al.
2004/0247268 A1	12/2004	Ishihara et al.	2008/0201081 A1	8/2008	Reid
2004/0254474 A1	12/2004	Seibel et al.	2008/0204762 A1	8/2008	Izatt et al.
2004/0258106 A1	12/2004	Araujo et al.	2008/0218696 A1	9/2008	Mir
			2008/0228086 A1	9/2008	Ilegbusi
			2008/0234560 A1	9/2008	Nomoto et al.
			2008/0265130 A1	10/2008	Colomb et al.
			2008/0308730 A1	12/2008	Vizi et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2009/0005691 A1 1/2009 Huang
 2009/0011948 A1 1/2009 Uniu et al.
 2009/0044799 A1 2/2009 Qiu
 2009/0051923 A1 2/2009 Zuluaga
 2009/0131801 A1 5/2009 Suter et al.
 2009/0192358 A1 7/2009 Jaffer et al.
 2009/0196477 A1 8/2009 Cense et al.
 2009/0209834 A1 8/2009 Fine
 2009/0273777 A1 11/2009 Yun et al.
 2009/0281390 A1 11/2009 Qiu et al.
 2009/0290156 A1 11/2009 Popescu et al.
 2009/0305309 A1 12/2009 Chien et al.
 2009/0323056 A1 12/2009 Yun et al.
 2010/0002241 A1 1/2010 Hirose
 2010/0086251 A1 4/2010 Xu et al.
 2010/0094576 A1 4/2010 de Boer et al.
 2010/0150467 A1 6/2010 Zhao et al.
 2010/0261995 A1 10/2010 Mckenna et al.
 2011/0028967 A1 2/2011 Rollins et al.
 2011/0160681 A1 6/2011 Dacey, Jr. et al.
 2011/0218403 A1 9/2011 Tearney et al.

FOREIGN PATENT DOCUMENTS

DE 19542955 5/1997
 DE 102005034443 2/2007
 EP 0110201 6/1984
 EP 0251062 1/1988
 EP 0617186 2/1994
 EP 0728440 8/1996
 EP 1324051 7/2003
 EP 1426799 6/2004
 FR 2738343 8/1995
 GB 2209221 5/1989
 GB 2298054 8/1996
 JP 6073405 4/1985
 JP 62-188001 6/1989
 JP 04-056907 2/1992
 JP 20040056907 2/1992
 JP 5509417 11/1993
 JP H8-136345 5/1996
 JP H08-160129 6/1996
 JP 9-230248 9/1997
 JP 10-213485 8/1998
 JP 10-267631 10/1998
 JP 10-267830 10/1998
 JP 2259617 10/1999
 JP 2000-023978 1/2000
 JP 2000-046729 2/2000
 JP 2000-121961 4/2000
 JP 2000-504234 4/2000
 JP 2000-126116 5/2000
 JP 2001-4447 1/2001
 JP 2001-500026 1/2001
 JP 2001-174404 6/2001
 JP 2001-174744 6/2001
 JP 2001-508340 6/2001
 JP 2007-539336 6/2001
 JP 2001-212086 8/2001
 JP 2008-533712 8/2001
 JP 2001-264246 9/2001
 JP 2001-525580 12/2001
 JP 2002-503134 1/2002
 JP 2002-035005 2/2002
 JP 2002-205434 2/2002
 JP 2002-095663 4/2002
 JP 2002-113017 4/2002
 JP 2002-148185 5/2002
 JP 2002-516586 6/2002
 JP 2002-214128 7/2002
 JP 2003-014585 1/2003
 JP 2003-504627 2/2003
 JP 20030035659 2/2003
 JP 2003-512085 4/2003

JP 2003-513278 4/2003
 JP 2003-216531 5/2003
 JP 2003-516531 5/2003
 JP 2004-028970 1/2004
 JP 2004-037165 2/2004
 JP 2004-057652 2/2004
 JP 2004-514920 5/2004
 JP 2004-258144 9/2004
 JP 2004-317437 11/2004
 JP 2005-062850 3/2005
 JP 2005-110208 4/2005
 JP 2005-156540 6/2005
 JP 2005-516187 6/2005
 JP 2005-195485 7/2005
 JP 2005-241872 9/2005
 JP 2006-237359 9/2006
 JP 2002214127 7/2007
 JP 2007271761 10/2007
 JP 2003-102672 4/2012
 RU 2149464 5/2000
 RU 2213421 9/2003
 RU 2255426 6/2005
 WO 7900841 10/1979
 WO 9201966 2/1992
 WO 9216865 10/1992
 WO 9219930 11/1992
 WO 9303672 3/1993
 WO 9533971 12/1995
 WO 96-02184 2/1996
 WO 96-04839 2/1996
 WO 9732182 9/1997
 WO 9800057 1/1998
 WO 9835203 8/1998
 WO 9848846 11/1998
 WO 9944089 2/1999
 WO 99-28856 6/1999
 WO 9944089 9/1999
 WO 99-45338 10/1999
 WO 9957507 11/1999
 WO 00-42906 7/2000
 WO 00-43730 7/2000
 WO 0058766 10/2000
 WO 01-04828 1/2001
 WO 0101111 1/2001
 WO 0127679 4/2001
 WO 01-33215 5/2001
 WO 0138820 5/2001
 WO 01-42735 6/2001
 WO 0142735 6/2001
 WO 01-82786 11/2001
 WO 02-37075 5/2002
 WO 0236015 5/2002
 WO 0237075 5/2002
 WO 0238040 5/2002
 WO 02-45572 6/2002
 WO 02-68853 6/2002
 WO 02053050 7/2002
 WO 02054027 7/2002
 WO 02-083003 10/2002
 WO 02084263 10/2002
 WO 03-003903 1/2003
 WO 03-012405 2/2003
 WO 03013624 2/2003
 WO 03020119 3/2003
 WO 03046495 6/2003
 WO 03046636 6/2003
 WO 03053226 7/2003
 WO 03062802 7/2003
 WO 03-088826 10/2003
 WO 03105678 12/2003
 WO 2004-037068 5/2004
 WO 2004-043251 5/2004
 WO 2004057266 7/2004
 WO 2004-073501 9/2004
 WO 2004-100789 11/2004
 WO 2004105598 12/2004
 WO 2005-045362 5/2005
 WO 2005-047813 5/2005
 WO 2005047813 5/2005

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO2005047813	*	5/2005	G01B 9/02
WO	2005082225		9/2005		
WO	2006004743		1/2006		
WO	2006-020605		2/2006		
WO	2006038876		4/2006		
WO	2006039091		4/2006		
WO	2006-050320		5/2006		
WO	2006-058187		6/2006		
WO	2006059109		6/2006		
WO	2006124860		11/2006		
WO	2006-131859		12/2006		
WO	2007-030835		3/2007		
WO	2007028531		3/2007		
WO	2007083138		7/2007		
WO	2007084995		7/2007		
WO	2009-033064		3/2009		
WO	2009153929		12/2009		
WO	2011-055376		5/2011		

OTHER PUBLICATIONS

- D. Huang et al., "Optical Coherence Tomography," *Science*, vol. 254, pp. 1178-1181, Nov. 1991.
- Tearney et al., "High-Speed Phase—and Group Delay Scanning with a Grating Based Phase Control Delay Line," *Optics Letters*, vol. 22, pp. 1811-1813, Dec. 1997.
- Rollins, et al., "In Vivo Video Rate Optical Coherence Tomography," *Optics Express*, vol. 3, pp. 219-229, Sep. 1998.
- Saxer, et al., High Speed Fiber-Based Polarization-Sensitive Optical Coherence Tomography of in Vivo Human Skin, *Optical Society of America*, vol. 25, pp. 1355-1357, Sep. 2000.
- Oscar Eduardo Martinez, "3000 Times Grating Compress or with Positive Group Velocity Dispersion," *IEEE*, vol. QE-23, pp. 59-64, Jan. 1987.
- Kulkarni, et al., "Image Enhancement in Optical Coherence Tomography Using Deconvolution," *Electronics Letters*, vol. 33, pp. 1365-1367, Jul. 1997.
- Bashkansky, et al., "Signal Processing for Improving Field Cross-Correlation Function in Optical Coherence Tomography," *Optics & Photonics News*, vol. 9, pp. 8137-8138, May 1998.
- Yung et al., "Phase-Domain Processing of Optical Coherence Tomography Images," *Journal of Biomedical Optics*, vol. 4, pp. 125-136, Jan. 1999.
- Tearney, et al., "In Vivo Endoscopic Optical Biopsy with Optical Coherence Tomography," *Science*, vol. 276, Jun. 1997.
- W. Drexler et al., "In Vivo Ultrahigh-Resolution Optical Coherence Tomography," *Optics Letters* vol. 24, pp. 1221-3, Sep. 1999.
- Nicuser V. Iftimia et al., "A Portable, Low Coherence Interferometry Based Instrument for Fine Needle Aspiration Biopsy Guidance," Accepted to Review of Scientific Instruments, 2005.
- Abbas, G.L., V.W.S. Chan et al., "Local-Oscillator Excess-Noise Suppression for Homodyne and Heterodyne-Detection," *Optics Letters*, vol. 8, pp. 419-421, Aug. 1983 issue.
- Agrawal, G.P., "Population Pulsations and Nondegenerate 4-Wave Mixing in Semiconductor-Lasers and Amplifiers," *Journal Of The Optical Society Of America B-Optical Physics*, vol. 5, pp. 147-159, Jan. 1998.
- Andretzky, P. et al., "Optical Coherence Tomography by Spectral Radar: Improvement of Signal-to-Noise Ratio," *The International Society for Optical Engineering, USA*, vol. 3915, 2000.
- Ballif, J. et al., "Rapid and Scalable Scans at 21 m/s in optical Low-Coherence Reflectometry," *Optics Letters*, vol. 22, pp. 757-759, Jun. 1997.
- Barfuss H. et al., "Modified Optical Frequency-Domain Reflectometry with High Spatial-Resolution for Components of Integrated Optic Systems," *Journal Of Lightwave Technology*, vol. 7, pp. 3-10, Jan. 1989.
- Beaud, P. et al., "Optical Reflectometry with Micrometer Resolution for the Investigation of Integrated Optical-Devices," *Lee Journal of Quantum Electronics*, vol. 25, pp. 755-759, Apr. 1989.

- Bouma, Brett et al., "Power-Efficient Nonreciprocal Interferometer and Linear-Scanning Fiber-Optic Catheter for Optical Coherence Tomography," *Optics Letters*, vol. 24, pp. 531-533, Apr. 1999.
- Brinkmeyer, E. et al., "Efficient Algorithm for Non-Equidistant Interpolation of Sampled Data," *Electronics Letters*, vol. 28, p. 693, Mar. 1992.
- Brinkmeyer, E. et al., "High-Resolution OCDR in Dispersive Wave-Guides," *Electronics Letters*, vol. 26, pp. 413-414, Mar. 1990.
- Chinn, S.R. et al., "Optical Coherence Tomography Using a Frequency-Tunable Optical Source," *Optics Letters*, vol. 22, pp. 340-342, Mar. 1997.
- Danielson, B.L. et al., "Absolute Optical Ranging Using Low Coherence Interferometry," *Applied Optics*, vol. 30, p. 2975, Jul. 1991.
- Dorrer, C. et al., "Spectral Resolution and Sampling Issues in Fourier-Transform Spectral Interferometry," *Journal of the Optical Society of America B-Optical Physics*, vol. 17, pp. 1795-1802, Oct. 2000.
- Dudley, J.M. et al., "Cross-Correlation Frequency Resolved Optical Gating Analysis of Broadband Continuum Generation in Photonic Crystal Fiber: Simulations and Experiments," *Optics Express*, vol. 10, p. 1215, Oct. 2002.
- Eickhoff, W. et al., "Optical Frequency-Domain Reflectometry in Single-Mode Fiber," *Applied Physics Letters*, vol. 39, pp. 693-695, 1981.
- Fercher, Adolf "Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 1, pp. 157-173, Apr. 1996.
- Ferreira, L.A. et al., "Polarization-Insensitive Fiberoptic White-Light Interferometry," *Optics Communications*, vol. 114, pp. 386-392, Feb. 1995.
- Fujii, Yohji, "High-Isolation Polarization-Independent Optical Circulator" *Journal of Lightwave Technology*, vol. 9, pp. 1239-1243, Oct. 1991.
- Glance, B., "Polarization Independent Coherent Optical Receiver," *Journal of Lightwave Technology*, vol. LT-5, p. 274, Feb. 1987.
- Glombitza, U., "Coherent Frequency-Domain Reflectometry for Characterization of Single-Mode Integrated-Optical Wave-Guides," *Journal of Lightwave Technology*, vol. 11, pp. 1377-1384, Aug. 1993.
- Golubovic, B. et al., "Optical Frequency-Domain Reflectometry Using Rapid Wavelength Tuning of a Cr⁴⁺:Forsterite Laser," *Optics Letters*, vol. 11, pp. 1704-1706, Nov. 1997.
- Haberland, U. H. P. et al., "Chirp Optical Coherence Tomography of Layered Scattering Media," *Journal of Biomedical Optics*, vol. 3, pp. 259-266, Jul. 1998.
- Hammer, Daniel X. et al., "Spectrally Resolved White-Light Interferometry for Measurement of Ocular Dispersion," *Journal of the Optical Society of America A-Optics Image Science and Vision*, vol. 16, pp. 2092-2102, Sep. 1999.
- Harvey, K. C. et al., "External-Cavity Diode-Laser Using a Grazing-Incidence Diffraction Grating," *Optics Letters*, vol. 16, pp. 910-912, Jun. 1991.
- Hausler, Gerd et al., "'Coherence Radar' and 'Spectral Radar' New Tools for Dermatological Diagnosis," *Journal of Biomedical Optics*, vol. 3, pp. 21-31, Jan. 1998.
- Hee, Michael R. et al., "Polarization-Sensitive Low-Coherence Reflectometer for Birefringence Characterization and Ranging," *Journal of the Optical Society of America B (Optical Physics)*, vol. 9, p. 903-908, Jun. 1992.
- Hotate Kazuo et al., "Optical Coherence Domain Reflectometry by Synthesis of Coherence Function," *Journal of Lightwave Technology*, vol. 11, pp. 1701-1710, Oct. 1993.
- Inoue, Kyo et al., "Nearly Degenerate 4-Wave-Mixing in a Traveling-Wave Semiconductor-Laser Amplifier," *Applied Physics Letters*, vol. 51, pp. 1051-1053, 1987.
- Ivanov, A. P. et al., "New Method for High-Range Resolution Measurements of Light Scattering in Optically Dense Inhomogeneous Media," *Optics Letters*, vol. 1, pp. 226-228, Dec. 1977.
- Ivanov, A. P. et al., "Interferometric Study of the Spatial Structure of a Light-Scattering Medium," *Journal of Applied Spectroscopy*, vol. 28, pp. 518-525, 1978.
- Kazovsky, L. G. et al., "Heterodyne Detection Through Rain, Snow, and Turbid Media: Effective Receiver Size at Optical Through Millimeter Wavelengths," *Applied Optics*, vol. 22, pp. 706-710, Mar. 1983

(56)

References Cited

OTHER PUBLICATIONS

- Kersey, A. D. et al., "Adaptive Polarization Diversity Receiver Configuration for Coherent Optical Fiber Communications," *Electronics Letters*, vol. 25, pp. 275-277, Feb. 1989.
- Kohlhaas, Andreas et al., "High-Resolution OADR for Testing Integrated-Optical Waveguides: Dispersion-Corrupted Experimental Data Corrected by a Numerical Algorithm," *Journal of Lightwave Technology*, vol. 9, pp. 1493-1502, Nov. 1991.
- Larkin, Kieran G., "Efficient Nonlinear Algorithm for Envelope Detection in White Light Interferometry," *Journal of the Optical Society of America A-Optics Image Science and Vision*, vol. 13, pp. 832-843, Apr. 1996.
- Leitgeb, R. et al., "Spectral measurement of Absorption by Spectroscopic Frequency-Domain Optical Coherence Tomography," *Optics Letters*, vol. 25, pp. 820-822, Jun. 2000.
- Lexer, F. et al., "Wavelength-Tuning Interferometry Distances," *Applied Optics*, vol. 36, pp. 6548-6553, Sep. 1997.
- Mitsui, Takahisa, "Dynamic Range of Optical Reflectometry with Spectral Interferometry," *Japanese Journal of Applied Physics Part 1-Regular Papers Short Notes & Review Papers*, vol. 38, pp. 6133-6137, 1999.
- Naganuma, Kazunori et al., "Group-Delay Measurement Using the Fourier-Transform of an Interferometric Cross-Correlation Generated by White Light," *Optics Letters*, vol. 15, pp. 393-395, Apr. 1990.
- Okoshi, Takanori, "Polarization-State Control Schemes for Heterodyne or Homodyne Optical Fiber Communications," *Journal of Lightwave Technology*, vol. LT-3, pp. 1232-1237, Dec. 1995.
- Passy, R. et al., "Experimental and Theoretical Investigations of Coherent OFDR with Semiconductor-Laser Sources," *Journal of Lightwave Technology*, vol. 12, pp. 1622-1630, Sep. 1994.
- Podoleanu, Adrian G., "Unbalanced Versus Balanced Operation in an Optical Coherence Tomography System," *Applied Optics*, vol. 39, pp. 173-182, Jan. 2000.
- Price, J. H. V. et al., "Tunable, Femtosecond Pulse Source Operating in the Range 1.06-1.33 μm Based on an Yb³⁺-doped Hole Fiber Amplifier," *Journal of the Optical Society of America B-Optical Physics*, vol. 19, pp. 1286-1294, Jun. 2002.
- Schmitt, J. M. et al., "Measurement of Optical-Properties of Biological Tissues By Low-Coherence Reflectometry," *Applied Optics*, vol. 32, pp. 6032-6042, Oct. 1993.
- Silberberg, Y. et al., "Passive-Mode Locking of a Semiconductor Diode-Laser," *Optics Letters*, vol. 9, pp. 507-509, Nov. 1984.
- Smith, L. Montgomery et al., "Absolute Displacement Measurements Using Modulation of the Spectrum of White-Light in a Michelson Interferometer," *Applied Optics*, vol. 28, pp. 3339-3342, Aug. 1989.
- Sonnenschein, C. M. et al., "Signal-To-Noise Relationships for Coaxial Systems that Heterodyne Backscatter from Atmosphere," *Applied Optics*, vol. 10, pp. 1600-1604, Jul. 1971.
- Sorin, W. V. et al., "Measurement of Rayleigh Backscattering at 1.55 μm with 32 μm Spatial Resolution," *IEEE Photonics Technology Letters*, vol. 4, pp. 374-376, Apr. 1992.
- Sorin, W. V. et al., "A Simple Intensity Noise-Reduction Technique for Optical Low-Coherence Reflectometry," *IEEE Photonics Technology Letters*, vol. 4, pp. 1404-1406, Dec. 1992.
- Swanson, E. A. et al., "High-Speed Optical Coherence Domain Reflectometry," *Optics Letters*, vol. 17, pp. 151-153, Jan. 1992.
- Takada, K. et al., "High-Resolution OFDR with Incorporated Fiberoptic Frequency Encoder," *IEEE Photonics Technology Letters*, vol. 4, pp. 1069-1072, Sep. 1992.
- Takada, Kazumasa et al., "Narrow-Band light source with Acoustooptic Tunable Filter for Optical Low-Coherence Reflectometry," *IEEE Photonics Technology Letters*, vol. 8, pp. 658-660, May 1996.
- Takada, Kazumasa et al., "New Measurement System for Fault Location in Optical Wave-Guide Devices Based on an Interferometric-Technique," *Applied Optics*, vol. 26, pp. 1603-1606, May 1987.
- Tateda, Mitsuhiro et al., "Interferometric Method for Chromatic Dispersion Measurement in a Single-Mode Optical Fiber," *IEEE Journal of Quantum Electronics*, vol. 17, pp. 404-407, Mar. 1981.
- Toide, M. et al., "Two-Dimensional Coherent Detection Imaging in Multiple Scattering Media Based the Directional Resolution Capability of the Optical Heterodyne Method," *Applied Physics B (Photophysics and Laser Chemistry)*, vol. B52, pp. 391-394, 1991.
- Trutna, W. R. et al., "Continuously Tuned External-Cavity Semiconductor-Laser," *Lightwave Technology*, vol. 11, pp. 1279-1286, Aug. 1993.
- Uttam, Deepak et al., "Precision Time Domain Reflectometry in Optical Fiber Systems Using a Frequency Modulated Continuous Wave Ranging Technique," *Journal of Lightwave Technology*, vol. 3, pp. 971-977, Oct. 1985.
- Von Der Weid, J. P. et al., "On the Characterization of Optical Fiber Network Components with Optical Frequency Domain Reflectometry," *Journal of Lightwave Technology*, vol. 15, pp. 1131-1141, Jul. 1997.
- Wysocki, P.F. et al., "Broad-Spectrum, Wavelength-Swept, Erbium-Doped Fiber Laser at 1.55- μm ," *Optics Letters*, vol. 15, pp. 879-881, Aug. 1990.
- Youngquist, Robert C. et al., "Optical Coherence-Domain Reflectometry—A New Optical Evaluation Technique," *Optics Letters*, vol. 12, pp. 158-160, Mar. 1987.
- Yun, S. H. et al., "Wavelength-Swept Fiber Laser with Frequency Shifted Feedback and Resonantly Swept Intra-Cavity Acoustooptic Tunable Filter," *IEEE Journal of Selected Topics in Quantum Electronics*, vol. 3, pp. 1087-1096, Aug. 1997.
- Yun, S. H. et al., "Interrogation of Fiber Grating Sensor Arrays with a Wavelength-Swept Fiber Laser," *Optics Letters*, vol. 23, pp. 843-845, Jun. 1998.
- Yung, K. M., "Phase-Domain Processing of Optical Coherence Tomography Images," *Journal of Biomedical Optics*, vol. 4, pp. 125-136, Jan. 1999.
- Zhou, Xiao-Qun et al., "Extended-Range FMCW Reflectometry Using an optical Loop with a Frequency Shifter," *IEEE Photonics Technology Letters*, vol. 8, pp. 248-250, Feb. 1996.
- Zorabedian, Paul et al., "Tuning Fidelity of Acoustooptically Controlled External Cavity Semiconductor-Lasers," *Journal of Lightwave Technology*, vol. 13, pp. 62-66, Jan. 1995.
- Victor S. Y. Lin et al., "A Porous Silicon-Based Optical Interferometric Biosensor," *Science Magazine*, vol. 278, pp. 840-843, Oct. 31, 1997.
- De Boer, Johannes F. et al., "Review of Polarization Sensitive Optical Coherence Tomography and Stokes Vector Determination," *Journal of Biomedical Optics*, vol. 7, No. 3, Jul. 2002, pp. 359-371.
- Jiao, Shuliang et al., "Depth-Resolved Two-Dimensional Stokes Vectors of Backscattered Light and Mueller Matrices of Biological Tissue Measured with Optical Coherence Tomography," *Applied Optics*, vol. 39, No. 34, Dec. 1, 2000, pp. 6318-6324.
- Park, B. Hyle et al., "In Vivo Burn Depth Determination by High-Speed Fiber-Based Polarization Sensitive Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 6 No. 4, Oct. 2001, pp. 474-479.
- Roth, Jonathan E. et al., "Simplified Method for Polarization-Sensitive Optical Coherence Tomography," *Optics Letters*, vol. 26, No. 14, Jul. 15, 2001, pp. 1069-1071.
- Hitzenberger, Christopher K. et al., "Measurement and Imaging of Birefringence and Optic Axis Orientation by Phase Resolved Polarization Sensitive Optical Coherence Tomography," *Optics Express*, vol. 9, No. 13, Dec. 17, 2001, pp. 780-790.
- Wang, Xueding et al., "Propagation of Polarized Light in Birefringent Turbid Media: Time-Resolved Simulations," Optical Imaging Laboratory, Biomedical Engineering Program, Texas A&M University.
- Wong, Brian J.F. et al., "Optical Coherence Tomography of the Rat Cochlea," *Biomedical Optics*, vol. 5, No. 4, Oct. 2000, pp. 367-370.
- Yao, Gang et al., "Propagation of Polarized Light in Turbid Media: Simulated Animation Sequences," *Optics Express*, vol. 7, No. 5, Aug. 28, 2000, pp. 198-203.
- Wang, Xiao-Jun et al., "Characterization of Dentin and Enamel by Use of Optical Coherence Tomography," *Applied Optics*, vol. 38, No. 10, Apr. 1, 1999, pp. 2092-2096.
- De Boer, Johannes F. et al., "Determination of the Depth-Resolved Stokes Parameters of Light Backscattered from Turbid Media by use

(56)

References Cited

OTHER PUBLICATIONS

- of Polarization-Sensitive Optical Coherence Tomography," *Optics Letters*, vol. 24, No. 5, Mar. 1, 1999, pp. 300-302.
- Ducros, Mathieu G. et al., "Polarization Sensitive Optical Coherence Tomography of the Rabbit Eye," *IEEE Journal of Selected Topics in Quantum Electronics*, vol. 5, No. 4, Jul./Aug. 1999, pp. 1159-1167.
- Groner, Warren et al., "Orthogonal Polarization Spectral Imaging: A New Method for Study of the Microcirculation," *Nature Medicine Inc.*, vol. 5 No. 10, Oct. 1999, pp. 1209-1213.
- De Boer, Johannes F. et al., "Polarization Effects in Optical Coherence Tomography of Various Viological Tissues," *IEEE Journal of Selected Topics in Quantum Electronics*, vol. 5, No. 4, Jul./Aug. 1999, pp. 1200-1204.
- Yao, Gang et al., "Two-Dimensional Depth-Resolved Mueller Matrix Characterization of Biological Tissue by Optical Coherence Tomography," *Optics Letters*, Apr. 15, 1999, vol. 24, No. 8, pp. 537-539.
- Lu, Shih-Yau et al., "Homogeneous and Inhomogeneous Jones Matrices," *J. Opt. Soc. Am. A.*, vol. 11, No. 2, Feb. 1994, pp. 766-773.
- Bickel, S. William et al., "Stokes Vectors, Mueller Matrices, and Polarized Scattered Light," *Am. J. Phys.*, vol. 53, No. 5, May 1985 pp. 468-478.
- Bréhonnet, F. Le Roy et al., "Optical Media and Target Characterization by Mueller Matrix Decomposition," *J. Phys. D: Appl. Phys.* 29, 1996, pp. 34-38.
- Cameron, Brent D. et al., "Measurement and Calculation of the Two-Dimensional Backscattering Mueller Matrix of a Turbid Medium," *Optics Letters*, vol. 23, No. 7, Apr. 1, 1998, pp. 485-487.
- De Boer, Johannes F. et al., "Two-Dimensional Birefringence Imaging in Biological Tissue by Polarization-Sensitive Optical Coherence Tomography," *Optics Letters*, vol. 22, No. 12, Jun. 15, 1997, pp. 934-936.
- De Boer, Johannes F. et al., "Imaging Thermally Damaged Tissue by Polarization Sensitive Optical Coherence Tomography," *Optics Express*, vol. 3, No. 6, Sep. 14, 1998, pp. 212-218.
- Everett, M.J. et al., "Birefringence Characterization of Biological Tissue by Use of Optical Coherence Tomography," *Optics Letters*, vol. 23, No. 3, Feb. 1, 1998, pp. 228-230.
- Hee, Michael R. et al., "Polarization-Sensitive Low-Coherence Reflectometer for Birefringence Characterization and Ranging," *J. Opt. Soc. Am. B.*, vol. 9, No. 6, Jun. 1992, pp. 903-908.
- Barakat, Richard, "Statistics of the Stokes Parameters," *J. Opt. Soc. Am. B.*, vol. 4, No. 7, Jul. 1987, pp. 1256-1263.
- Schmitt, J.M. et al., "Cross-Polarized Backscatter in Optical Coherence Tomography of Biological Tissue," *Optics Letters*, vol. 23, No. 13, Jul. 1, 1998, pp. 1060-1062.
- Schoenenberger, Klaus et al., "Mapping of Birefringence and Thermal Damage in Tissue by use of Polarization-Sensitive Optical Coherence Tomography," *Applied Optics*, vol. 37, No. 25, Sep. 1, 1998, pp. 6026-6036.
- Pierce, Mark C. et al., "Simultaneous Intensity, Birefringence, and Flow Measurements with High-Speed Fiber-Based Optical Coherence Tomography," *Optics Letters*, vol. 27, No. 17, Sep. 1, 2002, pp. 1534-1536.
- De Boer, Johannes F. et al., "Review of Polarization Sensitive Optical Coherence Tomography and Stokes Vector Determination," *Journal of Biomedical Optics*, Jul. 2002, vol. 7, No. 3, pp. 359-371.
- Fried, Daniel et al., "Imaging Caries Lesions and Lesion Progression with Polarization Sensitive Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 7, No. 4, Oct. 2002, pp. 618-627.
- Jiao, Shuliang et al., "Two-Dimensional Depth-Resolved Mueller Matrix of Biological Tissue Measured with Double-Beam Polarization-Sensitive Optical Coherence Tomography," *Optics Letters*, vol. 27, No. 2, Jan. 15, 2002, pp. 101-103.
- Jiao, Shuliang et al., "Jones-Matrix Imaging of Biological Tissues with Quadruple-Channel Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 7, No. 3, Jul. 2002, pp. 101-103.
- Kuranov, R.V. et al., "Complementary Use of Cross-Polarization and Standard OCT for Differential Diagnosis of Pathological Tissues," *Optics Express*, vol. 10, No. 15, Jul. 29, 2002, pp. 707-713.
- Cense, Barry et al., "In Vivo Depth-Resolved Birefringence Measurements of the Human Retinal Nerve Fiber Layer by Polarization-Sensitive Optical Coherence Tomography," *Optics Letters*, vol. 27, No. 18, Sep. 15, 2002, pp. 1610-1612.
- Ren, Hongwu et al., "Phase-Resolved Functional Optical Coherence Tomography: Simultaneous Imaging of In Situ Tissue Structure, Blood Flow Velocity, Standard Deviation, Birefringence, and Stokes Vectors in Human Skin," *Optics Letters*, vol. 27, No. 19, Oct. 1, 2002, pp. 1702-1704.
- Tripathi, Renu et al., "Spectral Shaping for Non-Gaussian Source Spectra in Optical Coherence Tomography," *Optics Letters*, vol. 27, No. 6, Mar. 15, 2002, pp. 406-408.
- Yasuno, Y. et al., "Birefringence Imaging of Human Skin by Polarization-Sensitive Spectral Interferometric Optical Coherence Tomography," *Optics Letters*, vol. 27, No. 20, Oct. 15, 2002 pp. 1803-1805.
- White, Brian R. et al., "In Vivo Dynamic Human Retinal Blood Flow Imaging Using Ultra-High-Speed Spectral Domain Optical Doppler Tomography," *Optics Express*, vol. 11, No. 25, Dec. 15, 2003, pp. 3490-3497.
- De Boer, Johannes F. et al., "Improved Signal-to-Noise Ratio in Spectral-Domain Compared with Time-Domain Optical Coherence Tomography," *Optics Letters*, vol. 28, No. 21, Nov. 1, 2003, pp. 2067-2069.
- Jiao, Shuliang et al., "Optical-Fiber-Based Mueller Optical Coherence Tomography," *Optics Letters*, vol. 28, No. 14, Jul. 15, 2003, pp. 1206-1208.
- Jiao, Shuliang et al., "Contrast Mechanisms in Polarization-Sensitive Mueller-Matrix Optical Coherence Tomography and Application in Burn Imaging," *Applied Optics*, vol. 42, No. 25, Sep. 1, 2003, pp. 5191-5197.
- Moreau, Julien et al., "Full-Field Birefringence Imaging by Thermal-Light Polarization-Sensitive Optical Coherence Tomography. I. Theory," *Applied Optics*, vol. 42, No. 19, Jul. 1, 2003, pp. 3800-3810.
- Moreau, Julien et al., "Full-Field Birefringence Imaging by Thermal-Light Polarization-Sensitive Optical Coherence Tomography. II. Instrument and Results," *Applied Optics*, vol. 42, No. 19, Jul. 1, 2003, pp. 3811-3818.
- Morgan, Stephen P. et al., "Surface-Reflection Elimination in Polarization Imaging of Superficial Tissue," *Optics Letters*, vol. 28, No. 2, Jan. 15, 2003, pp. 114-116.
- Oh, Jung-Taek et al., "Polarization-Sensitive Optical Coherence Tomography for Photoelasticity Testing of Glass/Epoxy Composites," *Optics Express*, vol. 11, No. 14, Jul. 14, 2003, pp. 1669-1676.
- Park, B. Hyle et al., "Real-Time Multi-Functional Optical Coherence Tomography," *Optics Express*, vol. 11, No. 7, Apr. 7, 2003, pp. 782-793.
- Shribak, Michael et al., "Techniques for Fast and Sensitive Measurements of Two-Dimensional Birefringence Distributions," *Applied Optics*, vol. 42, No. 16, Jun. 1, 2003, pp. 3009-3017.
- Somervell, A.R.D. et al., "Direct Measurement of Fringe Amplitude and Phase Using a Heterodyne Interferometer Operating in Broadband Light," *Elsevier, Optics Communications*, Oct. 2003.
- Stifter, D. et al., "Polarisation-Sensitive Optical Coherence Tomography for Material Characterisation and Strain-Field Mapping," *Applied Physics A 76, Materials Science & Processing*, Jan. 2003, pp. 947-951.
- Davé, Digant P. et al., "Polarization-Maintaining Fiber-Based Optical Low-Coherence Reflectometer for Characterization and Ranging of Birefringence," *Optics Letters*, vol. 28, No. 19, Oct. 1, 2003, pp. 1775-1777.
- Yang, Ying et al., "Observations of Birefringence in Tissues from Optic-Fibre-Based Optical Coherence Tomography," *Measurement Science and Technology*, Nov. 2002, pp. 41-46.
- Yun, S.H. et al., "High-Speed Optical Frequency-Domain Imaging," *Optics Express*, vol. 11, No. 22, Nov. 3, 2003, pp. 2953-2963.
- Yun, S.H. et al., "High-Speed Spectral-Domain Optical Coherence Tomography at 1.3 μm Wavelength," *Optics Express*, vol. 11, No. 26, Dec. 29, 2003, pp. 3598-3604.
- Zhang, Jun et al., "Determination of Birefringence and Absolute Optic Axis Orientation Using Polarization-Sensitive Optical Coherence Tomography with PM Fibers," *Optics Express*, vol. 11, No. 24, Dec. 1, 2003, pp. 3262-3270.

(56)

References Cited

OTHER PUBLICATIONS

- Pircher, Michael et al., "Three Dimensional Polarization Sensitive OCT of Human Skin In Vivo," 2004, *Optical Society of America*.
- Götzinger, Erich et al., "Measurement and Imaging of Birefringent Properties of the Human Cornea with Phase-Resolved, Polarization-Sensitive Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 9, No. 1, Jan./Feb. 2004, pp. 94-102.
- Guo, Shuguang et al., "Depth-Resolved Birefringence and Differential Optical Axis Orientation Measurements with Finer-based Polarization-Sensitive Optical Coherence Tomography," *Optics Letters*, vol. 29, No. 17, Sep. 1, 2004, pp. 2025-2027.
- Huang, Xiang-Run et al., "Variation of Peripapillary Retinal Nerve Fiber Layer Birefringence in Normal Human Subjects," *Investigative Ophthalmology & Visual Science*, vol. 45, No. 9, Sep. 2004, pp. 3073-3080.
- Matcher, Stephen J. et al., "The Collagen Structure of Bovine Intervertebral Disc Studied Using Polarization-Sensitive Optical Coherence Tomography," *Physics in Medicine and Biology*, 2004, pp. 1295-1306.
- Nassif, Nader et al., "In Vivo Human Retinal Imaging by Ultrahigh-Speed Spectral Domain Optical Coherence Tomography," *Optics Letters*, vol. 29, No. 5, Mar. 1, 2004, pp. 480-482.
- Nassif, N. A. et al., "In Vivo High-Resolution Video-Rate Spectral-Domain Optical Coherence Tomography of the Human Retina and Optic Nerve," *Optics Express*, vol. 12, No. 3, Feb. 9, 2004, pp. 367-376.
- Park, B. Hyle et al., "Comment on Optical-Fiber-Based Mueller Optical Coherence Tomography," *Optics Letters*, vol. 29, No. 24, Dec. 15, 2004, pp. 2873-2874.
- Park, B. Hyle et al., "Jones Matrix Analysis for a Polarization-Sensitive Optical Coherence Tomography System Using Fiber-Optic Components," *Optics Letters*, vol. 29, No. 21, Nov. 1, 2004, pp. 2512-2514.
- Pierce, Mark C. et al., "Collagen Denaturation can be Quantified in Burned Human Skin Using Polarization-Sensitive Optical Coherence Tomography," *Elsevier, Burns*, 2004, pp. 511-517.
- Pierce, Mark C. et al., "Advances in Optical Coherence Tomography Imaging Dermatology," *The Society for Investigative Dermatology, Inc.* 2004, pp. 458-463.
- Pierce, Mark C. et al., "Birefringence Measurements in Human Skin Using Polarization-Sensitive Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 9, No. 2, Mar./Apr. 2004, pp. 287-291.
- Cense, Barry et al., "In Vivo Birefringence and Thickness Measurements of the Human Retinal Nerve Fiber Layer Using Polarization-Sensitive Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 9, No. 1, Jan./Feb. 2004, pp. 121-125.
- Pircher, Michael et al., "Imaging of Polarization Properties of Human Retina in Vivo with Phase Resolved Transversal PS-OCT," *Optics Express*, vol. 12, No. 24, Nov. 29, 2004 pp. 5940-5951.
- Pircher, Michael et al., "Transversal Phase Resolved Polarization Sensitive Optical Coherence Tomography," *Physics in Medicine & Biology*, 2004, pp. 1257-1263.
- Srinivas, Shyam M. et al., "Determination of Burn Depth by Polarization-Sensitive Optical Coherence Tomography," *Journal of Biomedical Optics*, vol. 9, No. 1, Jan./Feb. 2004, pp. 207-212.
- Strasswimmer, John et al., "Polarization-Sensitive Optical Coherence Tomography of Invasive Basal Cell Carcinoma," *Journal of Biomedical Optics*, vol. 9, No. 2, Mar./Apr. 2004, pp. 292-298.
- Todorović, Miloš et al., "Determination of Local Polarization Properties of Biological Samples in the Presence of Diattenuation by use of Mueller Optical Coherence Tomography," *Optics Letters*, vol. 29, No. 20, Oct. 15, 2004, pp. 2402-2404.
- Yasuno, Yoshiaki et al., "Polarization-Sensitive Complex Fourier Domain Optical Coherence Tomography for Jones Matrix Imaging of Biological Samples," *Applied Physics Letters*, vol. 85, No. 15, Oct. 11, 2004, pp. 3023-3025.
- Acioli, L. H., M. Ulman, et al. (1991). "Femtosecond Temporal Encoding in Barium-Titanate." *Optics Letters* 16(24): 1984-1986.
- Aigouy, L., A. Lahrech, et al. (1999). "Polarization effects in apertureless scanning near-field optical microscopy: an experimental study." *Optics Letters* 24(4): 187-189.
- Akiba, M., K. P. Chan, et al. (2003). "Full-field optical coherence tomography by two-dimensional heterodyne detection with a pair of CCD cameras." *Optics Letters* 28(10): 816-818.
- Akkin, T., D. P. Dave, et al. (2004). "Detection of neural activity using phase-sensitive optical low-coherence reflectometry." *Optics Express* 12(11): 2377-2386.
- Akkin, T., D. P. Dave, et al. (2003). "Surface analysis using phase sensitive optical low coherence reflectometry." *Lasers in Surgery and Medicine*: 4-4.
- Akkin, T., D. P. Dave, et al. (2003). "Imaging tissue response to electrical and photothermal stimulation with nanometer sensitivity." *Lasers in Surgery and Medicine* 33(4): 219-225.
- Akkin, T., T. E. Milner, et al. (2002). "Phase-sensitive measurement of birefringence change as an indication of neural functionality and diseases." *Lasers in Surgery and Medicine*: 6-6.
- Andretzky, P., Lindner, M.W., Herrmann, J.M., Schultz, A., Konzog, M., Kiesewetter, F., Haeusler, G. (1999). "Optical coherence tomography by 'spectral radar': Dynamic range estimation and in vivo measurements of skin." *Proceedings of SPIE—The International Society Optical Engineering* 3567: pp. 78-87.
- Antcliff, R. J., T. J. ffytche, et al. (2000). "Optical coherence tomography of melanocytoma." *American Journal of Ophthalmology* 130(6): 845-7.
- Antcliff, R. J., M. R. Stanford, et al. (2000). "Comparison between optical coherence tomography and fundus fluorescein angiography for the detection of cystoid macular edema in patients with uveitis." *Ophthalmology* 107(3): 593-9.
- Anvari, B., T. E. Milner, et al. (1995). "Selective Cooling of Biological Tissues—Application For Thermally Mediated Therapeutic Procedures." *Physics in Medicine and Biology* 40(2): 241-252.
- Anvari, B., B. S. Tanenbaum, et al. (1995). "A Theoretical-Study of the Thermal Response of Skin to Cryogen Spray Cooling and Pulsed-Laser Irradiation—Implications for Treatment of Port-Wine Stain Birthmarks." *Physics in Medicine and Biology* 40(9): 1451-1465.
- Arend, O., M. Ruffer, et al. (2000). "Macular circulation in patients with diabetes mellitus with and without arterial hypertension." *British Journal of Ophthalmology* 84(12): 1392-1396.
- Arimoto, H. and Y. Ohtsuka (1997). "Measurements of the complex degree of spectral coherence by use of a wave-front-folded interferometer." *Optics Letters* 22(13): 958-960.
- Azzolini, C., F. Patelli, et al. (2001). "Correlation between optical coherence tomography data and biomicroscopic interpretation of idiopathic macular hole." *American Journal of Ophthalmology* 132(3): 348-55.
- Baba, T., K. Ohno-Matsui, et al. (2002). "Optical coherence tomography of choroidal neovascularization in high myopia." *Acta Ophthalmologica Scandinavica* 80(1): 82-7.
- Bail, M. A. H., Gerd; Herrmann, Juergen M.; Lindner, Michael W.; Ringler, R. (1996). "Optical coherence tomography with the "spectral radar": fast optical analysis in volume scatterers by short-coherence interferometry." *Proc. SPIE*, 2925: p. 298-303.
- Baney, D. M. and W. V. Sorin (1993). "Extended-Range Optical Low-Coherence Reflectometry Using a Recirculating Delay Technique." *Ieee Photonics Technology Letters* 5(9): 1109-1112.
- Baney, D. M., B. Szafraniec, et al. (2002). "Coherent optical spectrum analyzer." *Ieee Photonics Technology Letters* 14(3): 355-357.
- Barakat, R. (1981). "Bilinear Constraints between Elements of the 4by4 Mueller-Jones Transfer-Matrix of Polarization Theory." *Optics Communications* 38(3): 159-161.
- Barakat, R. (1993). "Analytic Proofs of the Arago-Fresnel Laws for the Interference of Polarized-Light." *Journal of the Optical Society of America a-Optics Image Science and Vision* 10(1): 180-185.
- Barbastathis, G. and D. J. Brady (1999). "Multidimensional tomographic imaging using volume holography." *Proceedings of the Ieee* 87(12): 2098-2120.
- Bardal, S., A. Kamal, et al. (1992). "Photoinduced Birefringence in Optical Fibers—a Comparative-Study of Low-Birefringence and High-Birefringence Fibers." *Optics Letters* 17(6): 411-413.

(56)

References Cited

OTHER PUBLICATIONS

- Barsky, S. H., S. Rosen, et al. (1980). "Nature and Evolution of Port Wine Stains—Computer-Assisted Study." *Journal of Investigative Dermatology* 74(3): 154-157.
- Barton, J. K., J. A. Izatt, et al. (1999). "Three-dimensional reconstruction of blood vessels from in vivo color Doppler optical coherence tomography images." *Dermatology* 198(4): 355-361.
- Barton, J. K., A. Rollins, et al. (2001). "Photothermal coagulation of blood vessels: a comparison of high-speed optical coherence tomography and numerical modelling." *Physics in Medicine and Biology* 46.
- Barton, J. K., A. J. Welch, et al. (1998). "Investigating pulsed dye laser-blood vessel interaction with color Doppler optical coherence tomography." *Optics Express* 3.
- Bashkansky, M., M. D. Duncan, et al. (1997). "Subsurface defect detection in ceramics by high-speed high-resolution optical coherent tomography." *Optics Letters* 22 (1):61-63.
- Bashkansky, M. and J. Reintjes (2000). "Statistics and reduction of speckle in optical coherence tomography." *Optics Letters* 25(8): 545-547.
- Baumgartner, A., S. Dichtl, et al. (2000). "Polarization-sensitive optical coherence tomography of dental structures." *Caries Research* 34(1): 59-69.
- Baumgartner, A., C. K. Hitzenberger, et al. (2000). "Resolution-improved dual-beam and standard optical coherence tomography: a comparison." *Graefes Archive for Clinical and Experimental Ophthalmology* 238(5): 385-392.
- Baumgartner, A., C. K. Hitzenberger, et al. (1998). "Signal and resolution enhancements in dual beam optical coherence tomography of the human eye." *Journal of Biomedical Optics* 3(1): 45-54.
- Beaurepaire, E., P. Gleyzes, et al. (1998). *Optical coherence microscopy for the in-depth study of biological structures: System based on a parallel detection scheme*, Proceedings of the SPIE—The International Society for Optical Engineering.
- Beaurepaire, E., L. Moreaux, et al. (1999). "Combined scanning optical coherence and two-photon-excited fluorescence microscopy." *Optics Letters* 24(14): 969-971.
- Bechara, F. G., T. Gambichler, et al. (2004). "Histomorphologic correlation with routine histology and optical coherence tomography." *Skin Research and Technology* 10 (3): 169-173.
- Bechmann, M., M. J. Thiel, et al. (2000). "Central corneal thickness determined with optical coherence tomography in various types of glaucoma. [see comments]." *British Journal of Ophthalmology* 84(11): 1233-7.
- Bek, T. and M. Kandi (2000). "Quantitative anomaloscopy and optical coherence tomography scanning in central serous chorioretinopathy." *Acta Ophthalmologica Scandinavica* 78(6): 632-7.
- Benoit, A. M., K. Naoun, et al. (2001). "Linear dichroism of the retinal nerve fiber layer expressed with Mueller matrices." *Applied Optics* 40(4): 565-569.
- Bicout, D., C. Brosseau, et al. (1994). "Depolarization of Multiply Scattered Waves by Spherical Diffusers—Influence of the Size Parameter." *Physical Review E* 49(2): 1767-1770.
- Blanchot, L., M. Lebec, et al. (1997). *Low-coherence in depth microscopy for biological tissues imaging: Design of a real time control system*. Proceedings of SPIE—The International Society for Optical Engineering.
- Blumenthal, E. Z. and R. N. Weinreb (2001). "Assessment of the retinal nerve fiber layer in clinical trials of glaucoma neuroprotection. [Review][36 refs]." *Survey of Ophthalmology* 45(Suppl 3): S305-12; discussion S332-4.
- Blumenthal, E. Z., J. M. Williams, et al. (2000). "Reproducibility of nerve fiber layer thickness measurements by use of optical coherence tomography." *Ophthalmology* 107(12): 2278-82.
- Boppart, S. A., B. E. Bouma, et al. (1996). "Imaging developing neural morphology using optical coherence tomography." *Journal of Neuroscience Methods* 70.
- Boppart, S. A., B. E. Bouma, et al. (1997). "Forward-imaging instruments for optical coherence tomography." *Optics Letters* 22.
- Boppart, S. A., B. E. Bouma, et al. (1998). "Intraoperative assessment of microsurgery with three-dimensional optical coherence tomography." *Radiology* 208: 81-86.
- Boppart, S. A., J. Herrmann, et al. (1999). "High-resolution optical coherence tomography-guided laser ablation of surgical tissue." *Journal of Surgical Research* 82(2): 275-84.
- Bouma, B. E. and J. G. Fujimoto (1996). "Compact Kerr-lens mode-locked resonators." *Optics Letters* 21.
- Bouma, B. E., L. E. Nelson, et al. (1998). "Optical coherence tomographic imaging of human tissue at 1.55 μm and 1.81 μm using Er and Tm-doped fiber sources." *Journal of Biomedical Optics* 3.
- Bouma, B. E., M. Ramaswamy-Paye, et al. (1997). "Compact resonator designs for mode-locked solid-state lasers." *Applied Physics B(Lasers and Optics)* B65.
- Bouma, B. E. and G. J. Tearney (2002). "Clinical imaging with optical coherence tomography." *Academic Radiology* 9(8): 942-953.
- Bouma, B. E., G. J. Tearney, et al. (1996). "Self-phase-modulated Kerr-lens mode-locked Cr:forsterite laser source for optical coherence tomography." *Optics Letters* 21(22): 1839.
- Bouma, B. E., G. J. Tearney, et al. (2000). "High-resolution imaging of the human esophagus and stomach in vivo using optical coherence tomography." *Gastrointestinal Endoscopy* 51(4): 467-474.
- Bouma, B. E., G. J. Tearney, et al. (2003). "Evaluation of intracoronary stenting by intravascular optical coherence tomography." *Heart* 89(3): 317-320.
- Bourquin, S., V. Monterosso, et al. (2000). "Video-rate optical low-coherence reflectometry based on a linear smart detector array." *Optics Letters* 25(2): 102-104.
- Bourquin, S., P. Seitz, et al. (2001). "Optical coherence tomography based on a two-dimensional smart detector array." *Optics Letters* 26(8): 512-514.
- Bouzid, A., M. A. G. Abushagur, et al. (1995). "Fiber-optic four-detector polarimeter." *Optics Communications* 118(3-4): 329-334.
- Bowd, C., R. N. Weinreb, et al. (2000). "The retinal nerve fiber layer thickness in ocular hypertensive, normal, and glaucomatous eyes with optical coherence tomography." *Archives of Ophthalmology* 118(1): 22-6.
- Bowd, C., L. M. Zangwill, et al. (2001). "Detecting early glaucoma by assessment of retinal nerve fiber layer thickness and visual function." *Investigative Ophthalmology & Visual Science* 42(9): 1993-2003.
- Bowd, C., L. M. Zangwill, et al. (2002). "Imaging of the optic disc and retinal nerve fiber layer: the effects of age, optic disc area, refractive error, and gender." *Journal of the Optical Society of America, A, Optics, Image Science, & Vision* 19(1): 197-207.
- Brand, S., J. M. Ponerros, et al. (2000). "Optical coherence tomography in the gastrointestinal tract." *Endoscopy* 32(10): 796-803.
- Brezinski, M. E. and J. G. Fujimoto (1999). "Optical coherence tomography: high-resolution imaging in nontransparent tissue." *IEEE Journal of Selected Topics in Quantum Electronics* 5(4): 1185-1192.
- Brezinski, M. E., G. J. Tearney, et al. (1996). "Imaging of coronary artery microstructure (in vitro) with optical coherence tomography." *American Journal of Cardiology* 77 (1): 92-93.
- Brezinski, M. E., G. J. Tearney, et al. (1996). "Optical coherence tomography for optical biopsy—Properties and demonstration of vascular pathology." *Circulation* 93(6): 1206-1213.
- Brezinski, M. E., G. J. Tearney, et al. (1997). "Assessing atherosclerotic plaque morphology: Comparison of optical coherence tomography and high frequency intravascular ultrasound." *Heart* 77(5): 397-403.
- Brink, H. B. K. and G. J. Vanbloklund (1988). "Birefringence of the Human Foveal Area Assessed In vivo with Mueller-Matrix Ellipsometry." *Journal of the Optical Society of America a-Optics Image Science and Vision* 5(1): 49-57.
- Brosseau, C. and D. Bicout (1994). "Entropy Production in Multiple-Scattering of Light by a Spatially Random Medium." *Physical Review E* 50(6): 4997-5005.
- Burgoyne, C. F., D. E. Mercante, et al. (2002). "Change detection in regional and volumetric disc parameters using longitudinal confocal scanning laser tomography." *Ophthalmology* 109(3): 455-66.

(56)

References Cited

OTHER PUBLICATIONS

- Candido, R. and T. J. Allen (2002). "Haemodynamics in microvascular complications in type 1 diabetes." *Diabetes-Metabolism Research and Reviews* 18(4): 286-304.
- Cense, B., T. C. Chen, et al. (2004). "Thickness and birefringence of healthy retinal nerve fiber layer tissue measured with polarization-sensitive optical coherence tomography." *Investigative Ophthalmology & Visual Science* 45(8): 2606-2612.
- Cense, B., N. Nassif, et al. (2004). "Ultrahigh-Resolution High-Speed Retinal Imaging Using Spectral-Domain Optical Coherence Tomography." *Optics Express* 12(11): 2435-2447.
- Chance, B., J. S. Leigh, et al. (1988). "Comparison of Time-Resolved and Time-Unresolved Measurements of Deoxyhemoglobin in Brain." *Proceedings of the National Academy of Sciences of the United States of America* 85(14): 4971-4975.
- Chang, E. P., D. A. Keedy, et al. (1974). "Ultrastructures of Rabbit Corneal Stroma—Mapping of Optical and Morphological Anisotropies." *Biochimica Et Biophysica Acta* 343(3): 615-626.
- Chartier, T., A. Hideur, et al. (2001). "Measurement of the elliptical birefringence of single-mode optical fibers." *Applied Optics* 40(30): 5343-5353.
- Chauhan, B. C., J. W. Blanchard, et al. (2000). "Technique for Detecting Serial Topographic Changes in the Optic Disc and Peripapillary Retina Using Scanning Laser Tomograph." *Invest Ophthalmol Vis Sci* 41: 775-782.
- Chen, Z. P., T. E. Milner, et al. (1997). "Optical Doppler tomographic imaging of fluid flow velocity in highly scattering media." *Optics Letters* 22(1): 64-66.
- Chen, Z. P., T. E. Milner, et al. (1997). "Noninvasive imaging of in vivo blood flow velocity using optical Doppler tomography." *Optics Letters* 22(14): 1119-1121.
- Chen, Z. P., Y. H. Zhao, et al. (1999). "Optical Doppler tomography." *Ieee Journal of Selected Topics in Quantum Electronics* 5(4): 1134-1142.
- Cheong, W. F., S. A. Prahl, et al. (1990). "A Review of the Optical Properties of Biological Tissues." *Ieee Journal of Quantum Electronics* 26(12): 2166-2185.
- Chernikov, S. V., Y. Zhu, et al. (1997). "Supercontinuum self-Q-switched ytterbium fiber laser." *Optics Letters* 22(5): 298-300.
- Cho, S. H., B. E. Bouma, et al. (1999). "Low-repetition-rate high-peak-power Kerr-lens mode-locked Ti:Al/sub 2/0/sub 3/ laser with a multiple-pass cavity." *Optics Letters* 24(6): 417-419.
- Choma, M. A., M. V. Sarunic, et al. (2003). "Sensitivity advantage of swept source and Fourier domain optical coherence tomography." *Optics Express* 11(18): 2183-2189.
- Choma, M. A., C. H. Yang, et al. (2003). "Instantaneous quadrature low-coherence interferometry with 3 x 3 fiber-optic couplers." *Optics Letters* 28(22): 2162-2164.
- Choplin, N. T. and D. C. Lundy (2001). "The sensitivity and specificity of scanning laser polarimetry in the detection of glaucoma in a clinical setting." *Ophthalmology* 108 (5): 899-904.
- Christens Barry, W. A., W. J. Green, et al. (1996). "Spatial mapping of polarized light transmission in the central rabbit cornea." *Experimental Eye Research* 62(6): 651-662.
- Chvapil, M., D. P. Speer, et al. (1984). "Identification of the depth of burn injury by collagen stainability." *Plastic & Reconstructive Surgery* 73(3): 438-41.
- Cioffi, G. A. (2001). "Three common assumptions about ocular blood flow and glaucoma." *Survey of Ophthalmology* 45: S325-S331.
- Coleman, A. L. (1999). "Glaucoma." *Lancet* 354(9192): 1803-10.
- Collaborative Normal-Tension Glaucoma Study Group (1998). "Comparison of Glaucomatous Progression Between Untreated Patients With Normal Tension Glaucoma and Patients with Therapeutically Reduced Intraocular Pressures." *Am J Ophthalmol* 126: 487-97.
- Collaborative Normal-Tension Glaucoma Study Group (1998). "The effectiveness of intraocular pressure reduction in the treatment of normal-tension glaucoma." *Am J Ophthalmol* 126: 498-505.
- Collaborative Normal-Tension Glaucoma Study Group (2001). "Natural History of Normal-Tension Glaucoma." *Ophthalmology* 108: 247-253.
- Colston, B. W., M. J. Everett, et al. (1998). "Imaging of hard- and soft-tissue structure in the oral cavity by optical coherence tomography." *Applied Optics* 37(16): 3582-3585.
- Colston, B. W., U. S. Sathyam, et al. (1998). "Dental OCT." *Optics Express* 3(6): 230-238.
- Congdon, N. G., D. S. Friedman, et al. (2003). "Important causes of visual impairment in the world today." *Jama—Journal of the American Medical Association* 290(15): 2057-2060.
- Cregan, R. F., B. J. Mangan, et al. (1999). "Single-mode photonic band gap guidance of light in air." *Science* 285(5433): 1537-1539.
- DalMolin, M., A. Galtarossa, et al. (1997). "Experimental investigation of linear polarization in high-birefringence single-mode fibers." *Applied Optics* 36(12): 2526-2528.
- Danielson, B. L. and C. D. Whittenberg (1987). "Guided-Wave Reflectometry with Micrometer Resolution." *Applied Optics* 26(14): 2836-2842.
- Dave, D. P. and T. E. Milner (2000). "Doppler-angle measurement in highly scattering media." *Optics Letters* 25(20): 1523-1525.
- de Boer, J. F., T. E. Milner, et al. (1998). *Two dimensional birefringence imaging in biological tissue using phase and polarization sensitive optical coherence tomography*. Trends in Optics and Photonics (TOPS): Advances in Optical Imaging and Photon Migration, Orlando, USA, Optical Society of America, Washington DC, 1998.
- de Boer, J. F., C. E. Saxer, et al. (2001). "Stable carrier generation and phase-resolved digital data processing in optical coherence tomography." *Applied Optics* 40(31): 5787-5790.
- Degroot, P. and L. Deck (1993). "3-Dimensional Imaging by Sub-Nyquist Sampling of White-Light Interferograms." *Optics Letters* 18(17): 1462-1464.
- Denk, W., J. H. Strickler, et al. (1990). "2-Photon Laser Scanning Fluorescence Microscopy." *Science* 248(4951): 73-76.
- Descour, M. R., A. H. O. Karkkainen, et al. (2002). "Toward the development of miniaturized Imaging systems for detection of precancer." *Ieee Journal of Quantum Electronics* 38(2): 122-130.
- Dettwiller, L. (1997). "Polarization state interference: A general investigation." *Pure and Applied Optics* 6(1): 41-53.
- DiCarlo, C. D., W. P. Roach, et al. (1999). "Comparison of optical coherence tomography imaging of cataracts with histopathology." *Journal of Biomedical Optics* 4.
- Ding, Z., Y. Zhao, et al. (2002). "Real-time phase-resolved optical coherence tomography and optical Doppler tomography." *Optics Express* 10(5): 236-245.
- Dobrin, P. B. (1996). "Effect of histologic preparation on the cross-sectional area of arterial rings." *Journal of Surgical Research* 61(2): 413-5.
- Donohue, D. J., B. J. Stoyanov, et al. (1995). "Numerical Modeling of the Corneas Lamellar Structure and Birefringence Properties." *Journal of the Optical Society of America a-Optics Image Science and Vision* 12(7): 1425-1438.
- Doornbos, R. M. P., R. Lang, et al. (1999). "The determination of in vivo human tissue optical properties and absolute chromophore concentrations using spatially resolved steady-state diffuse reflectance spectroscopy." *Physics in Medicine and Biology* 44(4): 967-981.
- Drexler, W., A. Baumgartner, et al. (1997). "Biometric investigation of changes in the anterior eye segment during accommodation." *Vision Research* 37(19): 2789-2800.
- Drexler, W., A. Baumgartner, et al. (1997). "Submicrometer precision biometry of the anterior segment of the human eye." *Investigative Ophthalmology & Visual Science* 38(7): 1304-1313.
- Drexler, W., A. Baumgartner, et al. (1998). "Dual beam optical coherence tomography: signal identification for ophthalmologic diagnosis." *Journal of Biomedical Optics* 3 (1): 55-65.
- Drexler, W., O. Findl, et al. (1998). "Partial coherence interferometry: A novel approach to biometry in cataract surgery." *American Journal of Ophthalmology* 126(4): 524-534.
- Drexler, W., O. Findl, et al. (1997). "Clinical feasibility of dual beam optical coherence topography and tomography for ophthalmologic diagnosis." *Investigative Ophthalmology & Visual Science* 38(4): 1038-1038.

(56)

References Cited

OTHER PUBLICATIONS

- Drexler, W., C. K. Hitzenberger, et al. (1998). "Investigation of dispersion effects in ocular media by multiple wavelength partial coherence interferometry." *Experimental Eye Research* 66(1): 25-33.
- Drexler, W., C. K. Hitzenberger, et al. (1996). "(Sub)micrometer precision biometry of the human eye by optical coherence tomography and topography." *Investigative Ophthalmology & Visual Science* 37(3): 4374-4374.
- Drexler, W., C. K. Hitzenberger, et al. (1995). "Measurement of the Thickness of Fundus Layers by Partial Coherence Tomography." *Optical Engineering* 34(3): 701-710.
- Drexler, W., U. Morgner, et al. (2001). "Ultrahigh-resolution ophthalmic optical coherence tomography." *Nature Medicine* 7(4): 502-507.
- Drexler, W., U. Morgner, et al. (2001). "Ultrahigh-resolution ophthalmic optical coherence tomography. [erratum appears in Nat Med May 2001;7(5):636.]" *Nature Medicine* 7(4): 502-7.
- Drexler, W., H. Sattmann, et al. (2003). "Enhanced visualization of macular pathology with the use of ultrahigh-resolution optical coherence tomography." *Archives of Ophthalmology* 121(5): 695-706.
- Drexler, W., D. Stamper, et al. (2001). "Correlation of collagen organization with polarization sensitive imaging of in vitro cartilage: implications for osteoarthritis." *Journal of Rheumatology* 28(6): 1311-8.
- Droog, E. J., W. Steenbergen, et al. (2001). "Measurement of depth of burns by laser Doppler perfusion imaging." *Burns* 27(6): 561-8.
- Dubois, A., K. Grieve, et al. (2004). "Ultrahigh-resolution full-field optical coherence tomography." *Applied Optics* 43(14): 2874-2883.
- Dubois, A., L. Vabre, et al. (2002). "High-resolution full-field optical coherence tomography with a Linnik microscope." *Applied Optics* 41(4): 805-812.
- Ducros, M., M. Laubscher, et al. (2002). "Parallel optical coherence tomography in scattering samples using a two-dimensional smart-pixel detector array." *Optics Communications* 202(1-3): 29-35.
- Ducros, M. G., J. D. Marsack, et al. (2001). "Primate retina imaging with polarization-sensitive optical coherence tomography." *Journal of the Optical Society of America a-Optics Image Science and Vision* 18(12): 2945-2956.
- Duncan, A., J. H. Meek, et al. (1995). "Optical Pathlength Measurements on Adult Head, Calf and Forearm and the Head of the Newborn-Infant Using Phase-Resolved Optical Spectroscopy." *Physics in Medicine and Biology* 40(2): 295-304.
- Eigensee, A., G. Haeusler, et al. (1996). "New method of short-coherence interferometry in human skin (in vivo) and in solid volume scatterers." *Proceedings of SPIE—The International Society for Optical Engineering* 2925: 169-178.
- Eisenbeiss, W., J. Marotz, et al. (1999). "Reflection-optical multispectral imaging method for objective determination of burn depth." *Burns* 25(8): 697-704.
- Elbaum, M., M. King, et al. (1972). "Wavelength-Diversity Technique for Reduction of Speckle Size." *Journal of the Optical Society of America* 62(5): 732-&.
- Ervin, J. C., H. G. Lemij, et al. (2002). "Clinician change detection viewing longitudinal stereophotographs compared to confocal scanning laser tomography in LSU Experimental the Glaucoma (LEG) Study." *Ophthalmology* 109(3): 467-81.
- Essenpreis, M., C. E. Elwell, et al. (1993). "Spectral Dependence of Temporal Point Spread Functions in Human Tissues." *Applied Optics* 32(4): 418-425.
- Eun, H. C. (1995). "Evaluation of skin blood flow by laser Doppler flowmetry. [Review] [151 refs]." *Clinics in Dermatology* 13(4): 337-47.
- Evans, J. A., J. M. Poneris, et al. (2004). "Application of a histopathologic scoring system to optical coherence tomography (OCT) images to identify high-grade dysplasia in Barrett's esophagus." *Gastroenterology* 126(4): A51-A51.
- Feldchtein, F. I., G. V. Gelikonov, et al. (1998). "In vivo OCT imaging of hard and soft tissue of the oral cavity." *Optics Express* 3(6): 239-250.
- Feldchtein, F. I., G. V. Gelikonov, et al. (1998). "Endoscopic applications of optical coherence tomography." *Optics Express* 3(6): 257-270.
- Fercher, A. F., W. Drexler, et al. (1997). "Optical ocular tomography." *Neuro-Ophthalmology* 18(2): 39-49.
- Fercher, A. F., W. Drexler, et al. (1994). *Measurement of optical distances by optical spectrum modulation*. Proceedings of SPIE—The International Society for Optical Engineering.
- Fercher, A. F., W. Drexler, et al. (2003). "Optical coherence tomography—principles and applications." *Reports on Progress in Physics* 66(2): 239-303.
- Fercher, A. F., C. Hitzenberger, et al. (1991). "Measurement of Intraocular Optical Distances Using Partially Coherent Laser-Light." *Journal of Modern Optics* 38(7): 1327-1333.
- Fercher, A. F., C. K. Hitzenberger, et al. (1996). *Ocular partial coherence interferometry*. Proceedings of SPIE—The International Society for Optical Engineering.
- Fercher, A. F., C. K. Hitzenberger, et al. (1993). "In-Vivo Optical Coherence Tomography." *American Journal of Ophthalmology* 116(1): 113-115.
- Fercher, A. F., C. K. Hitzenberger, et al. (1994). *In-vivo dual-beam optical coherence tomography*. Proceedings of SPIE—The International Society for Optical Engineering.
- Fercher, A. F., C. K. Hitzenberger, et al. (1995). "Measurement of Intraocular Distances by Backscattering Spectral Interferometry." *Optics Communications* 117(1-2): 43-48.
- Fercher, A. F., C. K. Hitzenberger, et al. (2000). "A thermal light source technique for optical coherence tomography." *Optics Communications* 185(1-3): 57-64.
- Fercher, A. F., C. K. Hitzenberger, et al. (2001). "Numerical dispersion compensation for Partial Coherence Interferometry and Optical Coherence Tomography." *Optics Express* 9(12): 610-615.
- Fercher, A. F., C. K. Hitzenberger, et al. (2002). "Dispersion compensation for optical coherence tomography depth-scan signals by a numerical technique." *Optics Communications* 204(1-6): 67-74.
- Fercher, A. F., H. C. Li, et al. (1993). "Slit Lamp Laser-Doppler Interferometer." *Lasers in Surgery and Medicine* 13(4): 447-452.
- Fercher, A. F., K. Mengedoh, et al. (1988). "Eye-Length Measurement by Interferometry with Partially Coherent-Light." *Optics Letters* 13(3): 186-188.
- Ferro, P., M. Haelterman, et al. (1991). "All-Optical Polarization Switch with Long Low-Birefringence Fiber." *Electronics Letters* 27(16): 1407-1408.
- Fetterman, M. R., D. Goswami, et al. (1998). "Ultrafast pulse shaping: amplification and characterization." *Optics Express* 3(10): 366-375.
- Findl, O., W. Drexler, et al. (2001). "Improved prediction of intraocular lens power using partial coherence interferometry." *Journal of Cataract and Refractive Surgery* 27 (6): 861-867.
- Fork, R. L., C. H. B. Cruz, et al. (1987). "Compression of Optical Pulses to 6 Femtoseconds by Using Cubic Phase Compensation." *Optics Letters* 12(7): 483-485.
- Foschini, G. J. and C. D. Poole (1991). "Statistical-Theory of Polarization Dispersion in Single-Mode Fibers." *Journal of Lightwave Technology* 9(11): 1439-1456.
- Francia, C., F. Bruyere, et al. (1998). "PMD second-order effects on pulse propagation in single-mode optical fibers." *Ieee Photonics Technology Letters* 10(12): 1739-1741.
- Fried, D., R. E. Glens, et al. (1995). "Nature of Light-Scattering in Dental Enamel and Dentin at Visible and near-Infrared Wavelengths." *Applied Optics* 34(7): 1278-1285.
- Fujimoto, J. G., M. E. Brezinski, et al. (1995). "Optical Biopsy and Imaging Using Optical Coherence Tomography." *Nature Medicine* 1(9): 970-972.
- Fukasawa, A. and H. Iijima (2002). "Optical coherence tomography of choroidal osteoma." *American Journal of Ophthalmology* 133(3): 419-21.
- Fymat, A. L. (1981). "High-Resolution Interferometric Spectrophotopolarimetry." *Optical Engineering* 20(1): 25-30.
- Galtarossa, A., L. Palmieri, et al. (2000). "Statistical characterization of fiber random birefringence." *Optics Letters* 25(18): 1322-1324.

(56)

References Cited

OTHER PUBLICATIONS

- Galtarossa, A., L. Palmieri, et al. (2000). "Measurements of beat length and perturbation length in long single-mode fibers." *Optics Letters* 25(6): 384-386.
- Gandjbakhche, A. H., P. Mills, et al. (1994). "Light-Scattering Technique for the Study of Orientation and Deformation of Red-Blood-Cells in a Concentrated Suspension." *Applied Optics* 33(6): 1070-1078.
- Garcia, N. and M. Nieto-Vesperinas (2002). "Left-handed materials do not make a perfect lens." *Physical Review Letters* 88(20).
- Gelikonov, V. M., G. V. Gelikonov, et al. (1995). "Coherent Optical Tomography of Microscopic Inhomogeneities in Biological Tissues." *Jetp Letters* 61(2): 158-162.
- George, N. and A. Jain (1973). "Speckle Reduction Using Multiple Tones of Illumination." *Applied Optics* 12(6): 1202-1212.
- Gibson, G. N., R. Klank, et al. (1996). "Electro-optically cavity-dumped ultrashort-pulse Ti:sapphire oscillator." *Optics Letters* 21(14): 1055.
- Gil, J. J. (2000). "Characteristic properties of Mueller matrices." *Journal of the Optical Society of America a-Optics Image Science and Vision* 17(2): 328-334.
- Gil, J. J. and E. Bernabeu (1987). "Obtainment of the Polarizing and Retardation Parameters of a Nondepolarizing Optical-System from the Polar Decomposition of Its Mueller Matrix." *Optik* 76(2): 67-71.
- Gladkova, N. D., G. A. Petrova, et al. (2000). "In vivo optical coherence tomography imaging of human skin: norm and pathology." *Skin Research and Technology* 6 (1): 6-16.
- Glaessl, A., A. G. Schreyer, et al. (2001). "Laser surgical planning with magnetic resonance imaging-based 3-dimensional reconstructions for intralesional Nd : YAG laser therapy of a venous malformation of the neck." *Archives of Dermatology* 137(10): 1331-1335.
- Gloesmann, M., B. Hermann, et al. (2003). "Histologic correlation of pig retina radial stratification with with ultrahigh-resolution optical coherence tomography." *Investigative Ophthalmology & Visual Science* 44(4): 1696-1703.
- Goldberg, L. and D. Mehuys (1994). "High-Power Superluminescent Diode Source." *Electronics Letters* 30(20): 1682-1684.
- Goldsmith, J. A., Y. Li, et al. (2005). "Anterior chamber width measurement by high speed optical coherence tomography." *Ophthalmology* 112(2): 238-244.
- Goldstein, L. E., J. A. Muffat, et al. (2003). "Cytosolic beta-amyloid deposition and supranuclear cataracts in lenses from people with Alzheimer's disease." *Lancet* 361(9365): 1258-1265.
- Golubovic, B., B. E. Bouma, et al. (1996). "Thin crystal, room-temperature Cr/sup 4 +/forstefite laser using near-infrared pumping." *Optics Letters* 21(24): 1993-1995.
- Gonzalez, S. and Z. Tannous (2002). "Real-time, in vivo confocal reflectance microscopy of basal cell carcinoma." *Journal of the American Academy of Dermatology* 47(6): 869-874.
- Gordon, M. O. and M. A. Kass (1999). "The Ocular Hypertension Treatment Study: design and baseline description of the participants." *Archives of Ophthalmology* 117(5): 573-83.
- Grayson, T. P., J. R. Torgerson, et al. (1994). "Observation of a Nonlocal Pancharatnam Phase-Shift in the Process of Induced Coherence without Induced Emission." *Physical Review A* 49(1): 626-628.
- Greaney, M. J., D. C. Hoffman, et al. (2002). "Comparison of optic nerve imaging methods to distinguish normal eyes from those with glaucoma." *Investigative Ophthalmology & Visual Science* 43(1): 140-5.
- Greenfield, D. S., H. Bagga, et al. (2003). "Macular thickness changes in glaucomatous optic neuropathy detected using optical coherence tomography." *Archives of Ophthalmology* 121(1): 41-46.
- Greenfield, D. S., R. W. Knighton, et al. (2000). "Effect of corneal polarization axis on assessment of retinal nerve fiber layer thickness by scanning laser polarimetry." *American Journal of Ophthalmology* 129(6): 715-722.
- Griffin, R. A., D. D. Sampson, et al. (1995). "Coherence Coding for Photonic Code-Division Multiple-Access Networks." *Journal of Lightwave Technology* 13(9): 1826-1837.
- Guedes, V., J. S. Schuman, et al. (2003). "Optical coherence tomography measurement of macular and nerve fiber layer thickness in normal and glaucomatous human eyes." *Ophthalmology* 110(1): 177-189.
- Gueugniaud, P. Y., H. Carsin, et al. (2000). "Current advances in the initial management of major thermal burns. [Review] [76 refs]." *Intensive Care Medicine* 26(7): 848-56.
- Guido, S. and R. T. Tranquillo (1993). "A Methodology for the Systematic and Quantitative Study of Cell Contact Guidance in Oriented Collagen Gels—Correlation of Fibroblast Orientation and Gel Birefringence." *Journal of Cell Science* 105: 317-331.
- Gurses-Ozden, R., H. Ishikawa, et al. (1999). "Increasing sampling density improves reproducibility of optical coherence tomography measurements." *Journal of Glaucoma* 8(4): 238-41.
- Guzzi, R. (1998). "Scattering Theory from Homogeneous and Coated Spheres." 1-11.
- Haberland, U. B., Vladimir; Schmitt, Hans J. (1996). "Optical coherent tomography of scattering media using electrically tunable near-infrared semiconductor laser." *Applied Optics* Draft Copy.
- Haberland, U. R., Walter; Blazek, Vladimir; Schmitt, Hans J. (1995). "Investigation of highly scattering media using near-infrared continuous wave tunable semiconductor laser." *Proc. SPIE*, 2389: 503-512.
- Hale, G. M. and M. R. Querry (1973). "Optical-Constants of Water in 200-Nm to 200-Mum Wavelength Region." *Applied Optics* 12(3): 555-563.
- Hammer, D. X., R. D. Ferguson, et al. (2002). "Image stabilization for scanning laser ophthalmoscopy." *Optics Express* 10(26): 1542.
- Hara, T., Y. Ooi, et al. (1989). "Transfer Characteristics of the Microchannel Spatial Light-Modulator." *Applied Optics* 28(22): 4781-4786.
- Harland, C. C., S. G. Kale, et al. (2000). "Differentiation of common benign pigmented skin lesions from melanoma by high-resolution ultrasound." *British Journal of Dermatology* 143(2): 281-289.
- Hartl, I., X. D. Li, et al. (2001). "Ultrahigh-resolution optical coherence tomography using continuum generation in an air-silica microstructure optical fiber." *Optics Letters* 26(9): 608-610.
- Hassenstein, A., A. A. Bialasiewicz, et al. (2000). "Optical coherence tomography in uveitis patients." *American Journal of Ophthalmology* 130(5): 669-70.
- Hattenhauer, M. G., D. H. Johnson, et al. (1998). "The probability of blindness from open-angle glaucoma. [see comments]." *Ophthalmology* 105(11): 2099-104.
- Hausler, G., J. M. Herrmann, et al. (1996). "Observation of light propagation in volume scatterers with 10(11)-fold slow motion." *Optics Letters* 21(14): 1087-1089.
- Hazebroek, H. F. and A. A. Holscher (1973). "Interferometric Ellipsometry." *Journal of Physics E—Scientific Instruments* 6(9): 822-826.
- Hazebroek, H. F. and W. M. Visser (1983). "Automated Laser Interferometric Ellipsometry and Precision Reflectometry." *Journal of Physics E—Scientific Instruments* 16(7): 654-661.
- He, Z. Y., N. Mukohzaka, et al. (1997). "Selective image extraction by synthesis of the coherence function using two-dimensional optical lock-in amplifier with microchannel spatial light modulator." *Ieee Photonics Technology Letters* 9(4): 514-516.
- Hee, M. R., J. A. Izatt, et al. (1993). "Femtosecond Transillumination Optical Coherence Tomography." *Optics Letters* 18(12): 950-952.
- Hee, M. R., J. A. Izatt, et al. (1995). "Optical coherence tomography of the human retina." *Archives of Ophthalmology* 113(3): 325-32.
- Hee, M. R., C. A. Puliafito, et al. (1998). "Topography of diabetic macular edema with optical coherence tomography." *Ophthalmology* 105(2): 360-70.
- Hee, M. R., C. A. Puliafito, et al. (1995). "Quantitative assessment of macular edema with optical coherence tomography." *Archives of Ophthalmology* 113(8): 1019-29.
- Hellmuth, T. and M. Welle (1998). "Simultaneous measurement of dispersion, spectrum, and distance with a fourier transform spectrometer." *Journal of Biomedical Optics* 3(1): 7-11.
- Hemenger, R. P. (1989). "Birefringence of a medium of tenuous parallel cylinders." *Applied Optics* 28(18): 4030-4034.

(56)

References Cited

OTHER PUBLICATIONS

- Henry, M. (1981). "Fresnel-Arago Laws for Interference in Polarized-Light—Demonstration Experiment." *American Journal of Physics* 49(7): 690-691.
- Herz, P. R., Y. Chen, et al. (2004). "Micromotor endoscope catheter for in vivo, ultrahigh-resolution optical coherence tomography." *Optics Letters* 29(19): 2261-2263.
- Hirakawa, H., H. Iijima, et al. (1999). "Optical coherence tomography of cystoid macular edema associated with retinitis pigmentosa." *American Journal of Ophthalmology* 128(2): 185-91.
- Hitzenberger, C. K., A. Baumgartner, et al. (1994). "Interferometric Measurement of Corneal Thickness with Micrometer Precision." *American Journal of Ophthalmology* 118(4): 468-476.
- Hitzenberger, C. K., A. Baumgartner, et al. (1999). "Dispersion effects in partial coherence interferometry: Implications for intraocular ranging." *Journal of Biomedical Optics* 4(1): 144-151.
- Hitzenberger, C. K., A. Baumgartner, et al. (1998). "Dispersion induced multiple signal peak splitting in partial coherence interferometry." *Optics Communications* 154 (4): 179-185.
- Hitzenberger, C. K., M. Danner, et al. (1999). "Measurement of the spatial coherence of superluminescent diodes." *Journal of Modern Optics* 46(12): 1763-1774.
- Hitzenberger, C. K. and A. F. Fercher (1999). "Differential phase contrast in optical coherence tomography." *Optics Letters* 24(9): 622-624.
- Hitzenberger, C. K., M. Sticker, et al. (2001). "Differential phase measurements in low-coherence interferometry without 2 pi ambiguity." *Optics Letters* 26(23): 1864-1866.
- Hoeling, B. M., A. D. Fernandez, et al. (2000). "An optical coherence microscope for 3-dimensional imaging in developmental biology." *Optics Express* 6(7): 136-146.
- Hoerauf, H., C. Scholz, et al. (2002). "Transscleral optical coherence tomography: a new imaging method for the anterior segment of the eye." *Archives of Ophthalmology* 120(6): 816-9.
- Hoffmann, K., M. Happe, et al. (1998). "Optical coherence tomography (OCT) in dermatology." *Journal of Investigative Dermatology* 110(4): 583-583.
- Hoh, S. T., D. S. Greenfield, et al. (2000). "Optical coherence tomography and scanning laser polarimetry in normal, ocular hypertensive, and glaucomatous eyes." *American Journal of Ophthalmology* 129(2): 129-35.
- Hohenleutner, U., M. Hilbert, et al. (1995). "Epidermal Damage and Limited Coagulation Depth with the Flashlamp-Pumped Pulsed Dye-Laser—a Histochemical-Study." *Journal of Investigative Dermatology* 104(5): 798-802.
- Holland, A. J. A., H. C. P. Martin, et al. (2002). "Laser Doppler imaging prediction of burn wound outcome in children." *Burns* 28(1): 11-17.
- Hotate, K. and T. Okugawa (1994). "Optical Information-Processing by Synthesis of the Coherence Function." *Journal of Lightwave Technology* 12(7): 1247-1255.
- Hourdakis, C. J. and A. Perris (1995). "A Monte-Carlo Estimation of Tissue Optical-Properties for Use in Laser Dosimetry." *Physics in Medicine and Biology* 40(3): 351-364.
- Hu, Z., F. Li, et al. (2000). "Wavelength-tunable narrow-linewidth semiconductor fiber-ring laser." *IEEE Photonics Technology Letters* 12(8):977-979.
- Huang, F., W. Yang, et al. (2001). "Quadrature spectral interferometric detection and pulse shaping." *Optics Letters* 6(6): 382-384.
- Huang, X. R. and R. W. Knighton (2002). "Linear birefringence of the retinal nerve fiber layer measured in vitro with a multispectral imaging micropolarimeter." *Journal of Biomedical Optics* 7(2): 199-204.
- Huber, R., M. Wojtkowski, et al. (2005). "Amplified, frequency swept lasers for frequency domain reflectometry and OCT imaging: design and scaling principles." *Optics Express* 13(9): 3513-3528.
- Hunter, D. G., J. C. Sandruck, et al. (1999). "Mathematical modeling of retinal birefringence scanning." *Journal of the Optical Society of America a-Optics Image Science and Vision* 16(9): 2103-2111.
- Hurwitz, H. H. and R. C. Jones (1941). "A new calculus for the treatment of optical systems II. Proof of three general equivalence theorems." *Journal of the Optical Society of America* 31(7): 493-499.
- Huttner, B., C. De Barros, et al. (1999). "Polarization-induced pulse spreading in birefringent optical fibers with zero differential group delay." *Optics Letters* 24(6): 370-372.
- Huttner, B., B. Gisin, et al. (1999). "Distributed PMD measurement with a polarization-OTDR in optical fibers." *Journal of Lightwave Technology* 17(10): 1843-1848.
- Huttner, B., J. Reecht, et al. (1998). "Local birefringence measurements in single-mode fibers with coherent optical frequency-domain reflectometry." *Ieee Photonics Technology Letters* 10(10): 1458-1460.
- Hyde, S. C. W., N. P. Barry, et al. (1995). "Sub-100-Mu-M Depth-Resolved Holographic Imaging through Scattering Media in the near-Infrared." *Optics Letters* 20(22): 2330-2332.
- Hyde, S. C. W., N. P. Barry, et al. (1995). "Depth-Resolved Holographic Imaging through Scattering Media by Photorefractive." *Optics Letters* 20(11): 1331-1333.
- Iftimia, N. V., B. E. Bouma, et al. (2004). "Adaptive ranging for optical coherence tomography." *Optics Express* 12(17): 4025-4034.
- Iida, T., N. Hagimura, et al. (2000). "Evaluation of central serous chorioretinopathy with optical coherence tomography." *American Journal of Ophthalmology* 129(1): 16-20.
- Imai, M., H. Iijima, et al. (2001). "Optical coherence tomography of tractional macular elevations in eyes with proliferative diabetic retinopathy. [republished in Am J Ophthalmol. Sep. 2001;132(3):458-61 ; 11530091.]" *American Journal of Ophthalmology* 132(1) 81-4.
- Indebetouw, G. and P. Klysubun (2000). "Imaging through scattering media with depth resolution by use of low-coherence gating in spatiotemporal digital holography." *Optics Letters* 25(4): 212-214.
- Ip, M. S., B. J. Baker, et al. (2002). "Anatomical outcomes of surgery for idiopathic macular hole as determined by optical coherence tomography." *Archives of Ophthalmology* 120(1): 29-35.
- Ismail, R., V. Tanner, et al. (2002). "Optical coherence tomography imaging of severe commotio retinae and associated macular hole." *British Journal of Ophthalmology* 86(4): 473-4.
- Izatt, J. A., M. R. Hee, et al. (1994). "Optical Coherence Microscopy in Scattering Media." *Optics Letters* 19(8): 590-592.
- Izatt, J. A., M. R. Hee, et al. (1994). "Micrometer-scale resolution imaging of the anterior eye in vivo with optical coherence tomography." *Archives of Ophthalmology* 112(12): 1584-9.
- Izatt, J. A., M. D. Kulkarni, et al. (1997). "In vivo bidirectional color Doppler flow imaging of picoliter blood volumes using optical coherence tomography." *Optics Letters* 22(18): 1439-1441.
- Izatt, J. A., M. D. Kulkarni, et al. (1996). "Optical coherence tomography and microscopy in gastrointestinal tissues." *IEEE Journal of Selected Topics in Quantum Electronics* 2(4): 1017.
- Jacques, S. L., J. S. Nelson, et al. (1993). "Pulsed Photothermal Radiometry of Port-Wine-Stain Lesions." *Applied Optics* 32(13): 2439-2446.
- Jacques, S. L., J. R. Roman, et al. (2000). "Imaging superficial tissues with polarized light." *Lasers in Surgery and Medicine* 26(2): 119-129.
- Jang, I. K., B. E. Bouma, et al. (2002). "Visualization of coronary atherosclerotic plaques in patients using optical coherence tomography: Comparison with intravascular ultrasound." *Journal of the American College of Cardiology* 39(4): 604-609.
- Jang, I. K., B. D. MacNeill, et al. (2002). "In-vivo characterization of coronary plaques in patients with ST elevation acute myocardial infarction using optical coherence tomography (OCT)." *Circulation* 106(19): 698-698 3440 Suppl. S.
- Jang, I. K., G. J. Tearney, et al. (2000). "Comparison of optical coherence tomography and intravascular ultrasound for detection of coronary plaques with large lipid-core in living patients." *Circulation* 102(18): 509-509.
- Jeng, J. C., A. Bridgeman, et al. (2003). "Laser Doppler imaging determines need for excision and grafting in advance of clinical judgment: a prospective blinded trial." *Burns* 29(7): 665-670.

(56)

References Cited

OTHER PUBLICATIONS

- Jesser, C. A., S. A. Boppart, et al. (1999). "High resolution imaging of transitional cell carcinoma with optical coherence tomography: feasibility for the evaluation of bladder pathology." *British Journal of Radiology* 72: 1170-1176.
- Johnson, C. A., J. L. Keltner, et al. (2002). "Baseline visual field characteristics in the ocular hypertension treatment study." *Ophthalmology* 109(3): 432-7.
- Jones, R. C. (1941). "A new calculus for the treatment of optical systems III. The Sohncke theory of optical activity." *Journal of the Optical Society of America* 31 (7): 500-503.
- Jones, R. C. (1941). "A new calculus for the treatment of optical systems I. Description and discussion of the calculus." *Journal of the Optical Society of America* 31(7): 488-493.
- Jones, R. C. (1942). "A new calculus for the treatment of optical systems. IV." *Journal of the Optical Society of America* 32(8): 486-493.
- Jones, R. C. (1947). "A New Calculus for the Treatment of Optical Systems .6. Experimental Determination of the Matrix." *Journal of the Optical Society of America* 37(2): 110-112.
- Jones, R. C. (1947). "A New Calculus for the Treatment of Optical Systems .5. A More General Formulation, and Description of Another Calculus." *Journal of the Optical Society of America* 37(2): 107-110.
- Jones, R. C. (1948). "A New Calculus for the Treatment of Optical Systems .7. Properties of the N-Matrices." *Journal of the Optical Society of America* 38(8): 671-685.
- Jones, R. C. (1956). "New Calculus for the Treatment of Optical Systems .8. Electromagnetic Theory." *Journal of the Optical Society of America* 46(2): 126-131.
- Jopson, R. M., L. E. Nelson, et al. (1999). "Measurement of second-order polarization-mode dispersion vectors in optical fibers." *Ieee Photonics Technology Letters* 11 (9): 1153-1155.
- Jost, B. M., A. V. Sergienko, et al. (1998). "Spatial correlations of spontaneously down-converted photon pairs detected with a single-photon-sensitive CCD camera." *Optics Express* 3(2): 81-88.
- Kaplan, B., E. Compain, et al. (2000). "Phase-modulated Mueller ellipsometry characterization of scattering by latex sphere suspensions." *Applied Optics* 39 (4): 629-636.
- Kass, M. A., D. K. Heuer, et al. (2002). "The Ocular Hypertension Treatment Study: a randomized trial determines that topical ocular hypotensive medication delays or prevents the onset of primary open-angle glaucoma." *Archives of Ophthalmology* 120(6): 701-13; discussion 829-30.
- Kasuga, Y., J. Arai, et al. (2000). "Optical coherence tomography to confirm early closure of macular holes." *American Journal of Ophthalmology* 130(5): 675-6.
- Kaufman, T., S. N. Lusthaus, et al. (1990). "Deep Partial Skin Thickness Burns—a Reproducible Animal-Model to Study Burn Wound-Healing." *Burns* 16(1): 13-16.
- Kemp, N. J., J. Park, et al. (2005). "High-sensitivity determination of birefringence in turbid media with enhanced polarization-sensitive optical coherence tomography." *Journal of the Optical Society of America a-Optics Image Science and Vision* 22(3): 552-560.
- Kerrigan-Baumrind, L. A., H. A. Quigley, et al. (2000). "Number of ganglion cells in glaucoma eyes compared with threshold visual field tests in the same persons." *Investigative Ophthalmology & Visual Science* 41(3): 741-8.
- Kesen, M. R., G. L. Spaeth, et al. (2002). "The Heidelberg Retina Tomograph vs clinical impression in the diagnosis of glaucoma." *American Journal of Ophthalmology* 133(5): 613-6.
- Kienle, A. and R. Hibst (1995). "A New Optimal Wavelength for Treatment of Port-Wine Stains." *Physics in Medicine and Biology* 40(10): 1559-1576.
- Kienle, A., L. Lilge, et al. (1996). "Spatially resolved absolute diffuse reflectance measurements for noninvasive determination of the optical scattering and absorption coefficients of biological tissue." *Applied Optics* 35(13): 2304-2314.
- Kim, B. Y. and S. S. Choi (1981). "Analysis and Measurement of Birefringence in Single-Mode Fibers Using the Backscattering Method." *Optics Letters* 6(11): 578-580.
- Kimel, S., L. O. Svaasand, et al. (1994). "Differential Vascular-Response to Laser Photothermolysis." *Journal of Investigative Dermatology* 103(5): 693-700.
- Kloppenber, F. W. H., G. Beerhuizen, et al. (2001). "Perfusion of burn wounds assessed by Laser Doppler Imaging is related to burn depth and healing time." *Burns* 27(4):359-363.
- Knighton, R. W. and X. R. Huang (2002). "Analytical methods for scanning laser polarimetry." *Optics Express* 10(21): 1179-1189.
- Knighton, R. W., X. R. Huang, et al. (2002). "Analytical model of scanning laser polarimetry for retinal nerve fiber layer assessment." *Investigative Ophthalmology & Visual Science* 43(2): 383-392.
- Knuettel, A. R. S., Joseph M.: Shay, M.; Knutson, Jay R. (1994). "Stationary low-coherence light imaging and spectroscopy using a CCD camera." *Proc. SPIE*, vol. 2135: 239-250.
- Knuttel, A. and M. Boehlau-Godau (2000). "Spatially confined and temporally resolved refractive index and scattering evaluation in human skin performed with optical coherence tomography." *Journal of Biomedical Optics* 5(1): 83-92.
- Knuttel, A. and J. M. Schmitt (1993). "Stationary Depth-Profiling Reflectometer Based on Low-Coherence Interferometry." *Optics Communications* 102(3-4): 193-198.
- Knuttel, A., J. M. Schmitt, et al. (1994). "Low-Coherence Reflectometry for Stationary Lateral and Depth Profiling with Acoustooptic Deflectors and a CCD Camera." *Optics Letters* 19(4): 302-304.
- Kobayashi, M., H. Hanafusa, et al. (1991). "Polarization-Independent Interferometric Optical-Time-Domain Reflectometer." *Journal of Lightwave Technology* 9(5): 623-628.
- Kolios, M. C., M. D. Sherar, et al. (1995). "Large Blood-Vessel Cooling in Heated Tissues—a Numerical Study." *Physics in Medicine and Biology* 40(4): 477-494.
- Koozekanani, D., K. Boyer, et al. (2001). "Retinal thickness measurements from optical coherence tomography using a Markov boundary model." *Ieee Transactions on Medical Imaging* 20(9): 900-916.
- Kop, R. H. J. and R. Sprik (1995). "Phase-sensitive interferometry with ultrashort optical pulses." *Review of Scientific Instruments* 66(12): 5459-5463.
- Kramer, R. Z., J. Bella, et al. (1999). "Sequence dependent conformational variations of collagen triple-helical structure." *Nature Structural Biology* 6(5): 454-7.
- Kulkarni, M. D., T. G. van Leeuwen, et al. (1998). "Velocity-estimation accuracy and frame-rate limitations in color Doppler optical coherence tomography." *Optics Letters* 23(13): 1057-1059.
- Kwon, Y. H., C. S. Kim, et al. (2001). "Rate of visual field loss and long-term visual outcome in primary open-angle glaucoma." *American Journal of Ophthalmology* 132(1): 47-56.
- Kwong, K. F., D. Yankelevich, et al. (1993). "400-Hz Mechanical Scanning Optical Delay-Line." *Optics Letters* 18(7): 558-560.
- Landers, J., I. Goldberg, et al. (2002). "Analysis of risk factors that may be associated with progression from ocular hypertension to primary open angle glaucoma." *Clin Experiment Ophthalmology* 30(4): 242-7.
- Laszlo, A. and A. Venetianer (1998). Heat resistance in mammalian cells: Lessons and challenges. *Stress of Life*. 851: 169-178.
- Laszlo, A. and A. Venetianer (1998). "Heat resistance in mammalian cells: lessons and challenges. [Review] [52 refs]." *Annals of the New York Academy of Sciences* 851: 169-78.
- Laufer, J., R. Simpson, et al. (1998). "Effect of temperature on the optical properties of ex vivo human dermis and subdermis." *Physics in Medicine and Biology* 43(9): 2479-2489.
- Lederer, D. E., J. S. Schuman, et al. (2003). "Analysis of macular volume in normal and glaucomatous eyes using optical coherence tomography." *American Journal of Ophthalmology* 135(6): 838-843.
- Lee, P. P., Z. W. Feldman, et al. (2003). "Longitudinal prevalence of major eye diseases." *Archives of Ophthalmology* 121(9): 1303-1310.
- Lehrer, M. S., T. T. Sun, et al. (1998). "Strategies of epithelial repair: modulation of stem cell and transit amplifying cell proliferation." *Journal of Cell Science* 111(Pt 19): 2867-75.

(56)

References Cited

OTHER PUBLICATIONS

- Leibowitz, H. M., D. E. Krueger, et al. (1980). "The Framingham Eye Study monograph: An ophthalmological and epidemiological study of cataract, glaucoma, diabetic retinopathy, macular degeneration, and visual acuity in a general population of 2631 adults, 1973-1975." *Survey of Ophthalmology* 24(Suppl): 335-610.
- Leitgeb, R., C. K. Hitzenberger, et al. (2003). "Performance of fourier domain vs. time domain optical coherence tomography." *Optics Express* 11(8): 889-894.
- Leitgeb, R., L. F. Schmetterer, et al. (2002). "Flow velocity measurements by frequency domain short coherence interferometry." *Proc. SPIE* 4619: 16-21.
- Leitgeb, R. A., W. Drexler, et al. (2004). "Ultrahigh resolution Fourier domain optical coherence tomography." *Optics Express* 12(10): 2156-2165.
- Leitgeb, R. A., C. K. Hitzenberger, et al. (2003). "Phase-shifting algorithm to achieve high-speed long-depth-range probing by frequency-domain optical coherence tomography." *Optics Letters* 28(22): 2201-2203.
- Leitgeb, R. A., L. Schmetterer, et al. (2003). "Real-time assessment of retinal blood flow with ultrafast acquisition by color Doppler Fourier domain optical coherence tomography." *Optics Express* 11(23): 3116-3121.
- Leitgeb, R. A., L. Schmetterer, et al. (2004). "Real-time measurement of in vitro flow by Fourier-domain color Doppler optical coherence tomography." *Optics Letters* 29 (2): 171-173.
- LeRoyBrehonnet, F. and B. LeJeune (1997). "Utilization of Mueller matrix formalism to obtain optical targets depolarization and polarization properties." *Progress in Quantum Electronics* 21(2): 109-151.
- Leske, M. C., A. M. Connell, et al. (1995). "Risk factors for open-angle glaucoma. The Barbados Eye Study. [see comments]." *Archives of Ophthalmology* 113(7): 918-24.
- Leske, M. C., A. M. Connell, et al. (2001). "Incidence of open-angle glaucoma: the Barbados Eye Studies. The Barbados Eye Studies Group. [see comments]." *Archives of Ophthalmology* 119(1): 89-95.
- Leske, M. C., A. Heijl, et al. (1999). "Early Manifest Glaucoma Trial. Design and Baseline Data." *Ophthalmology* 106(11): 2144-2153.
- Lewis, S. E., J. R. DeBoer, et al. (2005). "Sensitive, selective, and analytical improvements to a porous silicon gas sensor." *Sensors and Actuators B: Chemical* 110(1): 54-65.
- Lexer, F., C. K. Hitzenberger, et al. (1999). "Dynamic coherent focus OCT with depth-independent transversal resolution." *Journal of Modern Optics* 46(3): 541-553.
- Li, X., C. Chudoba, et al. (2000). "Imaging needle for optical coherence tomography." *Optics Letters* 25: 1520-1522.
- Li, X., T. H. Ko, et al. (2001). "Intraluminal fiber-optic Doppler imaging catheter for structural and functional optical coherence tomography." *Optics Letters* 26: 1906-1908.
- Liddington, M. I. and P. G. Shakespeare (1996). "Timing of the thermographic assessment of burns." *Burns* 22(1): 26-8.
- Lindmo, T., D. J. Smithies, et al. (1998). "Accuracy and noise in optical Doppler tomography studied by Monte Carlo simulation." *Physics in Medicine and Biology* 43(10): 3045-3064.
- Liu, J., X. Chen, et al. (1999). "New thermal wave aspects on burn evaluation of skin subjected to instantaneous heating." *IEEE Transactions on Biomedical Engineering* 46(4): 420-8.
- Luke, D. G., R. McBride, et al. (1995). "Polarization mode dispersion minimization in fiber-wound piezoelectric cylinders." *Optics Letters* 20(24): 2550-2552.
- MacNeill, B. D., I. K. Jang, et al. (2004). "Focal and multi-focal plaque distributions in patients with macrophage acute and stable presentations of coronary artery disease." *Journal of the American College of Cardiology* 44(5): 972-979.
- Mahgerefteh, D. and C. R. Menyuk (1999). "Effect of first-order PMD compensation on the statistics of pulse broadening in a fiber with randomly varying birefringence." *Ieee Photonics Technology Letters* 11(3): 340-342.
- Maitland, D. J. and J. T. Walsh, Jr. (1997). "Quantitative measurements of linear birefringence during heating of native collagen." *Lasers in Surgery & Medicine* 20 (3): 310-8.
- Majaron, B., S. M. Srinivas, et al. (2000). "Deep coagulation of dermal collagen with repetitive Er : YAG laser irradiation." *Lasers in Surgery and Medicine* 26(2): 215-222.
- Mansuripur, M. (1991). "Effects of High-Numerical-Aperture Focusing on the State of Polarization in Optical and Magneto-optic Data-Storage Systems." *Applied Optics* 30(22): 3154-3162.
- Marshall, G. W., S. J. Marshall, et al. (1997). "The dentin substrate: structure and properties related to bonding." *Journal of Dentistry* 25(6): 441-458.
- Martin, P. (1997). "Wound healing—Aiming for perfect skin regeneration." *Science* 276 (5309): 75-81.
- Martinez, O. E. (1987). "3000 Times Grating Compressor with Positive Group-Velocity Dispersion-Application to Fiber Compensation in 1.3-1.6 μ -M Region." *Ieee Journal of Quantum Electronics* 23(1): 59-64.
- Martinez, O. E., J. P. Gordon, et al. (1984). "Negative Group-Velocity Dispersion Using Refraction." *Journal of the Optical Society of America a-Optics Image Science and Vision* 1(10): 1003-1006.
- McKinney, J. D., M. A. Webster, et al. (2000). "Characterization and imaging in optically scattering media by use of laser speckle and a variable-coherence source." *Optics Letters* 25(1): 4-6.
- Miglior, S., M. Casula, et al. (2001). "Clinical ability of Heidelberg retinal tomograph examination to detect glaucomatous visual field changes." *Ophthalmology* 108 (9): 1621-7.
- Milner, T. E., D. M. Goodman, et al. (1996). "Imaging laser heated subsurface chromophores in biological materials: Determination of lateral physical dimensions." *Physics in Medicine and Biology* 41(1): 31-44.
- Milner, T. E., D. M. Goodman, et al. (1995). "Depth Profiling of Laser-Heated Chromophores in Biological Tissues by Pulsed Photothermal Radiometry." *Journal of the Optical Society of America a-Optics Image Science and Vision* 12 (7): 1479-1488.
- Milner, T. E., D. J. Smithies, et al. (1996). "Depth determination of chromophores in human skin by pulsed photothermal radiometry." *Applied Optics* 35(19): 3379-3385.
- Mishchenko, M. I. and J. W. Hovenier (1995). "Depolarization of Light Backscattered by Randomly Oriented Nonspherical Particles." *Optics Letters* 20(12): 1356-&.
- Mistlberger, A., J. M. Liebmann, et al. (1999). "Heidelberg retina tomography and optical coherence tomography in normal, ocular-hypertensive, and glaucomatous eyes." *Ophthalmology* 106(10): 2027-32.
- Mitsui, T. (1999). "High-speed detection of ballistic photons propagating through suspensions using spectral interferometry." *Japanese Journal of Applied Physics Part 1—Regular Papers Short Notes & Review Papers* 38(5A): 2978-2982.
- Molteno, A. C., N. J. Bosma, et al. (1999). "Otago glaucoma surgery outcome study: long-term results of trabeculectomy—1976 to 1995." *Ophthalmology* 106(9): 1742-50.
- Morgner, U., W. Drexler, et al. (2000). "Spectroscopic optical coherence tomography." *Optics Letters* 25(2): 111-113.
- Morgner, U., F. X. Kartner, et al. (1999). "Sub-two-cycle pulses from a Kerr-lens mode-locked Ti : sapphire laser (vol. 24, p. 411, 1999)." *Optics Letters* 24(13): 920-920.
- Mourant, J. R., A. H. Hielscher, et al. (1998). "Evidence of intrinsic differences in the light scattering properties of tumorigenic and nontumorigenic cells." *Cancer Cytopathology* 84(6): 366-374.
- Muller, M., J. Squier, et al. (1998). "Dispersion pre-compensation of 15 femtosecond optical pulses for high-numerical-aperture objectives." *Journal of Microscopy—Oxford* 191: 141-150.
- Muscat, S., N. McKay, et al. (2002). "Repeatability and reproducibility of corneal thickness measurements by optical coherence tomography." *Investigative Ophthalmology & Visual Science* 43(6): 1791-5.
- Musch, D. C., P. R. Lichter, et al. (1999). "The Collaborative Initial Glaucoma Treatment Study. Study Design, Methods, and Baseline Characteristics of Enrolled Patients." *Ophthalmology* 106: 653-662.
- Neerken, S., Lucassen, G.W., Bisschop, M.A., Lenderink, E., Nuijs, T.A.M. (2004). "Characterization of age-related effects in human skin: A comparative study that applies confocal laser scanning microscopy and optical coherence tomography." *Journal of Biomedical Optics* 9(2): 274-281.

(56)

References Cited

OTHER PUBLICATIONS

- Nelson, J. S., K. M. Kelly, et al. (2001). "Imaging blood flow in human port-wine stain in situ and in real time using optical Doppler tomography." *Archives of Dermatology* 137(6): 741-744.
- Newson, T. P., F. Farahi, et al. (1988). "Combined Interferometric and Polarimetric Fiber Optic Temperature Sensor with a Short Coherence Length Source." *Optics Communications* 68(3): 161-165.
- November, L. J. (1993). "Recovery of the Matrix Operators in the Similarity and Congruency Transformations—Applications in Polarimetry." *Journal of the Optical Society of America a-Optics Image Science and Vision* 10(4): 719-739.
- Oh, W. Y., S. H. Yun, et al. (2005). "Wide tuning range wavelength-swept laser with two semiconductor optical amplifiers." *Ieee Photonics Technology Letters* 17(3): 678-680.
- Oka, K. and T. Kato (1999). "Spectroscopic polarimetry with a channeled spectrum." *Optics Letters* 24(21): 1475-1477.
- Okugawa, T. and K. Rotate (1996). "Real-time optical image processing by synthesis of the coherence function using real-time holography." *Ieee Photonics Technology Letters* 8(2): 257-259.
- Oshima, M., R. Torii, et al. (2001). "Finite element simulation of blood flow in the cerebral artery." *Computer Methods in Applied Mechanics and Engineering* 191 (6-7): 661-671.
- Pan, Y. T., H. K. Xie, et al. (2001). "Endoscopic optical coherence tomography based on a microelectromechanical mirror." *Optics Letters* 26(24): 1966-1968.
- Parisi, V., G. Manni, et al. (2001). "Correlation between optical coherence tomography, pattern electroretinogram, and visual evoked potentials in open-angle glaucoma patients." *Ophthalmology* 108(5): 905-12.
- Park, B. H., M. C. Pierce, et al. (2005). "Real-time fiber-based multifunctional spectral-domain optical coherence tomography at 1.3 μm ." *Optics Express* 13(11): 3931-3944.
- Park, D. H., J. W. Hwang, et al. (1998). "Use of laser Doppler flowmetry for estimation of the depth of burns." *Plastic and Reconstructive Surgery* 101(6): 1516-1523.
- Pendry, J. B., A. J. Holden, et al. (1999). "Magnetism from conductors and enhanced nonlinear phenomena." *Ieee Transactions on Microwave Theory and Techniques* 47(11): 2075-2084.
- Penninckx, D. and V. Morenas (1999). "Jones matrix of polarization mode dispersion." *Optics Letters* 24(13): 875-877.
- Pierce, M. C., M. Shishkov, et al. (2005). "Effects of sample arm motion in endoscopic polarization-sensitive optical coherence tomography." *Optics Express* 13(15): 5739-5749.
- Pircher, M., E. Gotzinger, et al. (2003). "Measurement and imaging of water concentration in human cornea with differential absorption optical coherence tomography." *Optics Express* 11(18): 2190-2197.
- Pircher, M., E. Gotzinger, et al. (2003). "Speckle reduction in optical coherence tomography by frequency compounding." *Journal of Biomedical Optics* 8(3): 565-569.
- Podoleanu, A. G., G. M. Dobre, et al. (1998). "En-face coherence imaging using galvanometer scanner modulation." *Optics Letters* 23(3): 147-149.
- Podoleanu, A. G. and D. A. Jackson (1999). "Noise analysis of a combined optical coherence tomograph and a confocal scanning ophthalmoscope." *Applied Optics* 38(10): 2116-2127.
- Podoleanu, A. G., J. A. Rogers, et al. (2000). "Three dimensional OCT images from retina and skin." *Optics Express* 7(9): 292-298.
- Podoleanu, A. G., M. Seeger, et al. (1998). "Transversal and longitudinal images from the retina of the living eye using low coherence reflectometry." *Journal of Biomedical Optics* 3(1): 12-20.
- Poole, C. D. (1988). "Statistical Treatment of Polarization Dispersion in Single-Mode Fiber." *Optics Letters* 13(8): 687-689.
- Povazay, B., K. Bizheva, et al. (2002). "Submicrometer axial resolution optical coherence tomography." *Optics Letters* 27(20): 1800-1802.
- Qi, B., A. P. Himmer, et al. (2004). "Dynamic focus control in high-speed optical coherence tomography based on a microelectromechanical mirror." *Optics Communications* 232(1-6): 123-128.
- Radhakrishnan, S., A. M. Rollins, et al. (2001). "Real-time optical coherence tomography of the anterior segment at 1310 nm." *Archives of Ophthalmology* 119(8): 1179-1185.
- Rogers, A. J. (1981). "Polarization-Optical Time Domain Reflectometry—a Technique for the Measurement of Field Distributions." *Applied Optics* 20(6): 1060-1074.
- Rollins, A. M. and J. A. Izatt (1999). "Optimal interferometer designs for optical coherence tomography." *Optics Letters* 24(21): 1484-1486.
- Rollins, A. M., R. Ung-arunyawee, et al. (1999). "Real-time in vivo imaging of human gastrointestinal ultrastructure by use of endoscopic optical coherence tomography with a novel efficient interferometer design." *Optics Letters* 24(19): 1358-1360.
- Rollins, A. M., S. Yazdanfar, et al. (2002). "Real-time in vivo colors Doppler optical coherence tomography." *Journal of Biomedical Optics* 7(1): 123-129.
- Rollins, A. M., S. Yazdanfar, et al. (2000). "Imaging of human retinal hemodynamics using color Doppler optical coherence tomography." *Investigative Ophthalmology & Visual Science* 41(4): S548-S548.
- Sandoz, P. (1997). "Wavelet transform as a processing tool in white-light interferometry." *Optics Letters* 22(14): 1065-1067.
- Sankaran, V., M. J. Everett, et al. (1999). "Comparison of polarized-light propagation in biological tissue and phantoms." *Optics Letters* 24(15): 1044-1046.
- Sankaran, V., J. T. Walsh, et al. (2000). "Polarized light propagation through tissue phanto, ehms containing densely packed scatterers." *Optics Letters* 25(4): 239-241.
- Sarunic, M. V., M. A. Choma, et al. (2005). "Instantaneous complex conjugate resolved spectral domain and swept-source OCT using 3x3 fiber couplers." *Optics Express* 13(3): 957-967.
- Sathyam, U. S., B. W. Colston, et al. (1999). "Evaluation of optical coherence quantitation of analytes in turbid media by use of two wavelengths." *Applied Optics* 38(10): 2097-2104.
- Schmitt, J. M. (1997). "Array detection for speckle reduction in optical coherence microscopy." *Physics in Medicine and Biology* 42(7): 1427-1439.
- Schmitt, J. M. (1999). "Optical coherence tomography (OCT): A review." *Ieee Journal of Selected Topics in Quantum Electronics* 5(4): 1205-1215.
- Schmitt, J. M. and A. Knüttel (1997). "Model of optical coherence tomography of heterogeneous tissue." *Journal of the Optical Society of America a-Optics Image Science and Vision* 14(6): 1231-1242.
- Schmitt, J. M., S. L. Lee, et al. (1997). "An optical coherence microscope with enhanced resolving power in thick tissue." *Optics Communications* 142(4-6): 203-207.
- Schmitt, J. M., S. H. Xiang, et al. (1998). "Differential absorption imaging with optical coherence tomography." *Journal of the Optical Society of America a-Optics Image Science and Vision* 15(9): 2288-2296.
- Schmitt, J. M., S. H. Xiang, et al. (1999). "Speckle in optical coherence tomography." *Journal of Biomedical Optics* 4(1): 95-105.
- Schmitt, J. M., M. J. Yadlowsky, et al. (1995). "Subsurface Imaging of Living Skin with Optical Coherence Microscopy." *Dermatology* 191(2): 93-98.
- Shi, H., J. Finlay, et al. (1997). "Multiwavelength 10-GHz picosecond pulse generation from a single-stripe semiconductor diode laser." *Ieee Photonics Technology Letters* 9(11): 1439-1441.
- Shi, H., I. Nitta, et al. (1999). "Demonstration of phase correlation in multiwavelength mode-locked semiconductor diode lasers." *Optics Letters* 24(4): 238-240.
- Simon, R. (1982). "The Connection between Mueller and Jones Matrices of Polarization Optics." *Optics Communications* 42(5): 293-297.
- Smith, P. J. M., E.M.; Taylor, C.M.; Selviah, D.R.; Day, S.E.; Commander, L.G. "Variable-Focus Microlenses as a Potential Technology for Endoscopy."
- Smithies, D. J., T. Lindmo, et al. (1998). "Signal attenuation and localization in optical coherence tomography studied by Monte Carlo simulation." *Physics in Medicine and Biology* 43(10): 3025-3044.
- Sorin, W. V. and D. F. Gray (1992). "Simultaneous Thickness and Group Index Measurement Using Optical Low-Coherence Reflectometry." *Ieee Photonics Technology Letters* 4(1): 105-107.

(56)

References Cited

OTHER PUBLICATIONS

- Sticker, M., C. K. Hitzengerger, et al. (2001). "Quantitative differential phase measurement and imaging in transparent and turbid media by optical coherence tomography." *Optics Letters* 26(8): 518-520.
- Sticker, M., M. Pircher, et al. (2002). "En face imaging of single cell layers by differential phase-contrast optical coherence microscopy." *Optics Letters* 27(13): 1126-1128.
- Stoller, P., B. M. Kim, et al. (2002). "Polarization-dependent optical second-harmonic imaging of a rat-tail tendon." *Journal of Biomedical Optics* 7(2): 205-214.
- Sun, C. S. (2003). "Multiplexing of fiber-optic acoustic sensors in a Michelson interferometer configuration." *Optics Letters* 28(12): 1001-1003.
- Swanson, E. A., J. A. Izatt, et al. (1993). "In-Vivo Retinal Imaging by Optical Coherence Tomography." *Optics Letters* 18(21): 1864-1866.
- Takada, K., A. Himeno, et al. (1991). "Phase-Noise and Shot-Noise Limited Operations of Low Coherence Optical-Time Domain Reflectometry." *Applied Physics Letters* 59(20): 2483-2485.
- Takenaka, H. (1973). "Unified Formalism for Polarization Optics by Using Group-Theory I (Theory)." *Japanese Journal of Applied Physics* 12(2): 226-231.
- Tanno, N., T. Ichimura, et al. (1994). "Optical Multimode Frequency-Domain Reflectometer." *Optics Letters* 19(8): 587-589.
- Tan-no, N., T. Ichimura, et al. (1994). "Optical Multimode Frequency-Domain Reflectometer." *Optics Letters* 19(8): 587-589.
- Targowski, P., M. Wojtkowski, et al. (2004). "Complex spectral OCT in human eye imaging in vivo." *Optics Communications* 229(1-6): 79-84.
- Tearney, G. J., S. A. Boppart, et al. (1996). "Scanning single-mode fiber optic catheter-endoscope for optical coherence tomography (vol. 21, p. 543, 1996)." *Optics Letters* 21(12): 912-912.
- Tearney, G. J., B. E. Bouma, et al. (1996). "Rapid acquisition of in vivo biological images by use of optical coherence tomography." *Optics Letters* 21(17): 1408-1410.
- Tearney, G. J., B. E. Bouma, et al. (1997). "In vivo endoscopic optical biopsy with optical coherence tomography." *Science* 276(5321): 2037-2039.
- Tearney, G. J., M. E. Brezinski, et al. (1996). "Catheter-based optical imaging of a human coronary artery." *Circulation* 94(11): 3013-3013.
- Tearney, G. J., M. E. Brezinski, et al. (1997). "In vivo endoscopic optical biopsy with optical coherence tomography." *Science* 276(5321): 2037-9.
- Tearney, G. J., M. E. Brezinski, et al. (1997). "Optical biopsy in human gastrointestinal tissue using optical coherence tomography." *American Journal of Gastroenterology* 92(10): 1800-1804.
- Tearney, G. J., M. E. Brezinski, et al. (1995). "Determination of the refractive index of highly scattering human tissue by optical coherence tomography." *Optics Letters* 20(21): 2258-2260.
- Tearney, G. J., I. K. Jang, et al. (2000). "Porcine coronary imaging in vivo by optical coherence tomography." *Acta Cardiologica* 55(4): 233-237.
- Tearney, G. J., R. H. Webb, et al. (1998). "Spectrally encoded confocal microscopy." *Optics Letters* 23(15): 1152-1154.
- Tearney, G. J., H. Yabushita, et al. (2003). "Quantification of macrophage content in atherosclerotic plaques by optical coherence tomography." *Circulation* 107(1): 113-119.
- Tower, T. T. and R. T. Tranquillo (2001). "Alignment maps of tissues: I. Microscopic elliptical polarimetry." *Biophysical Journal* 81(5): 2954-2963.
- Tower, T. T. and R. T. Tranquillo (2001). "Alignment maps of tissues: II. Fast harmonic analysis for imaging." *Biophysical Journal* 81(5): 2964-2971.
- Troy, T. L. and S. N. Thennadil (2001). "Optical properties of human skin in the near infrared wavelength range of 1000 to 2200 nm." *Journal of Biomedical Optics* 6 (2): 167-176.
- Vabre, L., A. Dubois, et al. (2002). "Thermal-light full-field optical coherence tomography." *Optics Letters* 27(7): 530-532.
- Vakhtin, A. B., D. J. Kane, et al. (2003). "Common-path interferometer for frequency-domain optical coherence tomography." *Applied Optics* 42(34): 6953-6958.
- Vakhtin, A. B., K. A. Peterson, et al. (2003). "Differential spectral interferometry: an imaging technique for biomedical applications." *Optics Letters* 28(15): 1332-1334.
- Vakoc, B. J., S. H. Yun, et al. (2005). "Phase-resolved optical frequency domain imaging." *Optics Express* 13(14): 5483-5493.
- van Leeuwen, T. G., M. D. Kulkarni, et al. (1999). "High-flow-velocity and shear-rate imaging by use of color Doppler optical coherence tomography." *Optics Letters* 24(22): 1584-1586.
- Vansteenkiste, N., P. Vignolo, et al. (1993). "Optical Reversibility Theorems for Polarization—Application to Remote-Control of Polarization." *Journal of the Optical Society of America a-Optics Image Science and Vision* 10(10): 2240-2245.
- Vargas, O., E. K. Chan, et al. (1999). "Use of an agent to reduce scattering in skin." *Lasers in Surgery and Medicine* 24(2): 133-141.
- Wang, R. K. (1999). "Resolution improved optical coherence-gated tomography for imaging through biological tissues." *Journal of Modern Optics* 46(13): 1905-1912.
- Wang, X. J., T. E. Milner, et al. (1997). "Measurement of fluid-flow-velocity profile in turbid media by the use of optical Doppler tomography." *Applied Optics* 36(1): 144-149.
- Wang, X. J., T. E. Milner, et al. (1995). "Characterization of Fluid-Flow Velocity by Optical Doppler Tomography." *Optics Letters* 20(11): 1337-1339.
- Wang, Y. M., J. S. Nelson, et al. (2003). "Optimal wavelength for ultrahigh-resolution optical coherence tomography." *Optics Express* 11(12): 1411-1417.
- Wang, Y. M., Y. H. Zhao, et al. (2003). "Ultrahigh-resolution optical coherence tomography by broadband continuum generation from a photonic crystal fiber." *Optics Letters* 28(3): 182-184.
- Watkins, L. R., S. M. Tan, et al. (1999). "Determination of interferometer phase distributions by use of wavelets." *Optics Letters* 24(13): 905-907.
- Wetzel, J. (2001). "Optical coherence tomography in dermatology: a review." *Skin Research and Technology* 7(1): 1-9.
- Wentworth, R. H. (1989). "Theoretical Noise Performance of Coherence-Multiplexed Interferometric Sensors." *Journal of Lightwave Technology* 7(6): 941-956.
- Westphal, V., A. M. Rollins, et al. (2002). "Correction of geometric and refractive image distortions in optical coherence tomography applying Fermat's principle." *Optics Express* 10(9): 397-404.
- Westphal, V., S. Yazdanfar, et al. (2002). "Real-time, high velocity-resolution color Doppler optical coherence tomography." *Optics Letters* 27(1): 34-36.
- Williams, P. A. (1999). "Rotating-wave-plate Stokes polarimeter for differential group delay measurements of polarization-mode dispersion." *Applied Optics* 38(31): 6508-6515.
- Wojtkowski, M., T. Bajraszewski, et al. (2003). "Real-time in vivo imaging by high-speed spectral optical coherence tomography." *Optics Letters* 28(19): 1745-1747.
- Wojtkowski, M., A. Kowalczyk, et al. (2002). "Full range complex spectral optical coherence tomography technique in eye imaging." *Optics Letters* 27(16): 1415-1417.
- Wojtkowski, M., R. Leitgeb, et al. (2002). "In vivo human retinal imaging by Fourier domain optical coherence tomography." *Journal of Biomedical Optics* 7(3): 457-463.
- Wojtkowski, M., R. Leitgeb, et al. (2002). "Fourier domain OCT imaging of the human eye in vivo." *Proc. SPIE* 4619: 230-236.
- Wojtkowski, M., V. J. Srinivasan, et al. (2004). "Ultrahigh-resolution, high-speed, Fourier domain optical coherence tomography and methods for dispersion compensation." *Optics Express* 12(11): 2404-2422.
- Wong, B. J. F., Y. H. Zhao, et al. (2004). "Imaging the internal structure of the rat cochlea using optical coherence tomography at 0.827 μm and 1.3 μm ." *Otolaryngology-Head and Neck Surgery* 130(3): 334-338.
- Yabushita, H. B., B. E.; Houser, S. L.; Aretz, H. T.; Jang, I.; Schlendorf, K. H.; Kauffman, C. R.; Shishkov, M.; Halpern, E. F.; Tearney, G. J. "Measurement of Thin Fibrous Caps in Atherosclerotic Plaques by Optical Coherence Tomography."

(56)

References Cited

OTHER PUBLICATIONS

- Yang, C., A. Wax, et al. (2001). "Phase-dispersion optical tomography." *Optics Letters* 26(10): 686-688.
- Yang, C., A. Wax, et al. (2001). "Phase-referenced interferometer with subwavelength and subhertz sensitivity applied to the study of cell membrane dynamics." *Optics Letters* 26(16): 1271-1273.
- Yang, C. H., A. Wax, et al. (2001). "Phase-dispersion optical tomography." *Optics Letters* 26(10): 686-688.
- Yang, C. H., A. Wax, et al. (2000). "Interferometric phase-dispersion microscopy." *Optics Letters* 25(20): 1526-1528.
- Yang, V. X. D., M. L. Gordon, et al. (2002). "Improved phase-resolved optical Doppler tomography using the Kasai velocity estimator and histogram segmentation." *Optics Communications* 208(4-6): 209-214.
- Yang, V. X. D., M. L. Gordon, et al. (2003). "High speed, wide velocity dynamic range Doppler optical coherence tomography (Part I): System design, signal processing, and performance." *Optics Express* 11(7): 794-809.
- Yang, V. X. D., M. L. Gordon, et al. (2003). "High speed, wide velocity dynamic range Doppler optical coherence tomography (Part II): Imaging in vivo cardiac dynamics of *Xenopus laevis*." *Optics Express* 11(14): 1650-1658.
- Yang, V. X. D., M. L. Gordon, et al. (2003). "High speed, wide velocity dynamic range Doppler optical coherence tomography (Part III): in vivo endoscopic imaging of blood flow in the rat and human gastrointestinal tracts." *Optics Express* 11(19): 2416-2424.
- Yang, V. X. D., B. Qi, et al. (2003). "In vivo feasibility of endoscopic catheter-based Doppler optical coherence tomography." *Gastroenterology* 124(4): A49-A50.
- Yao, G. and L. H. V. Wang (2000). "Theoretical and experimental studies of ultrasound-modulated optical tomography in biological tissue." *Applied Optics* 39(4): 659-664.
- Yazdanfar, S. and J. A. Izatt (2002). "Self-referenced Doppler optical coherence tomography." *Optics Letters* 27(23): 2085-2087.
- Yazdanfar, S., M. D. Kulkarni, et al. (1997). "High resolution imaging of in vivo cardiac dynamics using color Doppler optical coherence tomography." *Optics Express* 1 (13) : 424-431.
- Yazdanfar, S., A. M. Rollins, et al. (2000). "Imaging and velocimetry of the human retinal circulation with color Doppler optical coherence tomography." *Optics Letters* 25(19): 1448-1450.
- Yazdanfar, S., A. M. Rollins, et al. (2000). "Noninvasive imaging and velocimetry of human retinal blood flow using color Doppler optical coherence tomography." *Investigative Ophthalmology & Visual Science* 41(4): S548-S548.
- Yazdanfar, S., A. M. Rollins, et al. (2003). "In vivo imaging of human retinal flow dynamics by color Doppler optical coherence tomography." *Archives of Ophthalmology* 121(2): 410-416.
- Yazdanfar, S., C. H. Yang, et al. (2005). "Frequency estimation precision in Doppler optical coherence tomography using the Cramer-Rao lower bound." *Optics Express* 13(2): 410-416.
- Yun, S. H., C. Boudoux, et al. (2004). "Extended-cavity semiconductor wavelength-swept laser for biomedical imaging." *Ieee Photonics Technology Letters* 16(1): 293-295.
- Yun, S. H., C. Boudoux, et al. (2003). "High-speed wavelength-swept semiconductor laser with a polygon-scanner-based wavelength filter." *Optics Letters* 28(20): 1981-1983.
- Yun, S. H., G. J. Tearney, et al. (2004). "Pulsed-source and swept-source spectral-domain optical coherence tomography with reduced motion artifacts." *Optics Express* 12(23): 5614-5624.
- Yun, S. H., G. J. Tearney, et al. (2004). "Removing the depth-degeneracy in optical frequency domain imaging with frequency shifting." *Optics Express* 12(20): 4822-4828.
- Yun, S. H., G. J. Tearney, et al. (2004). "Motion artifacts in optical coherence tomography with frequency-domain ranging." *Optics Express* 12(13): 2977-2998.
- Zhang, J., J. S. Nelson, et al. (2005). "Removal of a mirror image and enhancement of the signal-to-noise ratio in Fourier-domain optical coherence tomography using an electro-optic phase modulator." *Optics Letters* 30(2): 147-149.
- Zhang, Y., M. Sato, et al. (2001). "Numerical investigations of optimal synthesis of several low coherence sources for resolution improvement." *Optics Communications* 192(3-6): 183-192.
- Zhang, Y., M. Sato, et al. (2001). "Resolution improvement in optical coherence tomography by optimal synthesis of light-emitting diodes." *Optics Letters* 26(4): 205-207.
- Zhao, Y., Z. Chen, et al. (2002). "Real-time phase-resolved functional optical coherence tomography by use of optical Hilbert transformation." *Optics Letters* 27(2): 98-100.
- Zhao, Y. H., Z. P. Chen, et al. (2000). "Doppler standard deviation imaging for clinical monitoring of in vivo human skin blood flow." *Optics Letters* 25(18): 1358-1360.
- Zhao, Y. H., Z. P. Chen, et al. (2000). "Phase-resolved optical coherence tomography and optical Doppler tomography for imaging blood flow in human skin with fast scanning speed and high velocity sensitivity." *Optics Letters* 25(2): 114-116.
- Zhou, D., P. R. Prucnal, et al. (1998). "A widely tunable narrow linewidth semiconductor fiber ring laser." *IEEE Photonics Technology Letters* 10(6): 781-783.
- Zuluaga, A. F. and R. Richards-Kortum (1999). "Spatially resolved spectral interferometry for determination of subsurface structure." *Optics Letters* 24(8): 519-521.
- Zvyagin, A. V., J. B. FitzGerald, et al. (2000). "Real-time detection technique for Doppler optical coherence tomography." *Optics Letters* 25(22): 1645-1647.
- Marc Nikles et al., "Brillouin gain spectrum characterization in single-mode optical fibers", *Journal of Lightwave Technology* 1997, 15 (10): 1842-1851.
- Tsuyoshi Sonehara et al., "Forced Brillouin Spectroscopy Using Frequency-Tunable Continuous-Wave Lasers", *Physical Review Letters* 1995, 75 (23): 4234-4237.
- Hajime Tanaka et al., "New Method of Superheterodyne Light Beating Spectroscopy for Brillouin-Scattering Using Frequency-Tunable Lasers", *Physical Review Letters* 1995, 74 (9): 1609-1612.
- Webb RH et al. "Confocal Scanning Laser Ophthalmoscope", *Applied Optics* 1987, 26 (8): 1492-1499.
- Andreas Zumbusch et al. "Three-dimensional vibrational imaging by coherent anti-Stokes Raman scattering", *Physical Review Letters* 1999, 82 (20): 4142-4145.
- Katrin Kneipp et al., "Single molecule detection using surface-enhanced Raman scattering (SERS)", *Physical Review Letters* 1997, 78 (9): 1667-1670.
- K.J. Koski et al., "Brillouin imaging" *Applied Physics Letters* 87, 2005.
- Boas et al., "Diffusing temporal light correlation for burn diagnosis", *SPIE*, 1999, 2979:468-477.
- David J. Briers, "Speckle fluctuations and biomedical optics: implications and applications", *Optical Engineering*, 1993, 32(2):277-283.
- Clark et al., "Tracking Speckle Patterns with Optical Correlation", *SPIE*, 1992, 1772:77-87.
- Clark et al., "Tracking Speckle Patterns with Optical Correlation", *SPIE*, 1992, 1772:77-87.
- Facchini et al., "An endoscopic system for DSPI", *Optik*, 1993, 95(1):27-30.
- Hrabovsky, M., "Theory of speckle displacement and decorrelation: application in mechanics", *SPIE*, 1998, 3479:345-354.
- Sean J. Kirkpatrick et al., "Micromechanical behavior of cortical bone as inferred from laser speckle data", *Journal of Biomedical Materials Research*, 1998, 39(3):373-379.
- Sean J. Kirkpatrick et al., "Laser speckle microstrain measurements in vascular tissue", *SPIE*, 1999, 3598:121-129.
- Loree et al., "Mechanical Properties of Model Atherosclerotic Lesion Lipid Pools", *Arteriosclerosis and Thrombosis*, 1994, 14(2):230-234.
- Podbielska, H. "Interferometric Methods and Biomedical Research", *SPIE*, 1999, 2732:134-141.
- Richards-Kortum et al., "Spectral diagnosis of atherosclerosis using an optical fiber laser catheter", *American Heart Journal*, 1989, 118(2):381-391.
- Ruth, B. "blood flow determination by the laser speckle method", *Int J Microcirc: Clin Exp*, 1990, 9:21-45.

(56)

References Cited

OTHER PUBLICATIONS

- Shapo et al., "Intravascular strain imaging: Experiments on an Inhomogeneous Phantom", *IEEE Ultrasonics Symposium* 1996, 2:1177-1180.
- Shapo et al., "Ultrasonic displacement and strain imaging of coronary arteries with a catheter array", *IEEE Ultrasonics Symposium* 1995, 2:1511-1514.
- Thompson et al., "Imaging in scattering media by use of laser speckle", *Opt. Soc. Am. A.*, 1997, 14(9):2269-2277.
- Thompson et al., "Diffusive media characterization with laser speckle", *Applied Optics*, 1997, 36(16):3726-3734.
- Tuchin, Valery V., "Coherent Optical Techniques for the Analysis of Tissue Structure and Dynamics," *Journal of Biomedical Optics*, 1999, 4(1):106-124.
- M. Wussling et al., "Laser diffraction and speckling studies in skeletal and heart muscle", *Biomed. Biochim. Acta*, 1986, 45(1/2):S 23-S 27.
- T. Yoshimura et al., "Statistical properties of dynamic speckles", *J. Opt. Soc. Am. A.* 1986, 3(7):1032-1054.
- Zimnyakov et al., "Spatial speckle correlometry in applications to tissue structure monitoring", *Applied Optics* 1997, 36(22): 5594-5607.
- Zimnyakov et al., "A study of statistical properties of partially developed speckle fields as applied to the diagnosis of structural changes in human skin", *Optics and Spectroscopy*, 1994, 76(5): 747-753.
- Zimnyakov et al., "Speckle patterns polarization analysis as an approach to turbid tissue structure monitoring", *SPIE* 1999, 2981:172-180.
- Ramasamy Manoharan et al., "Biochemical analysis and mapping of atherosclerotic human artery using FT-IR microspectroscopy", *Atherosclerosis*, May 1993, 181-1930.
- N. V. Salunke et al., "Biomechanics of Atherosclerotic Plaque" *Critical Reviews™ in Biomedical Engineering* 1997, 25(3):243-285.
- D. Fu et al., "Non-invasive quantitative reconstruction of tissue elasticity using an iterative forward approach", *Phys. Med. Biol.* 2000 (45): 1495-1509.
- S.B. Adams Jr. et al., "The use of polarization sensitive optical coherence tomography and elastography to assess connective tissue", *Optical Soc. Of American Washington* 2002, p. 3.
- International Search Report for International Patent application No. PCT/US2005/039740.
- International Written Opinion for International Patent application No. PCT/US2005/039740.
- International Search Report for International Patent application No. PCT/US2005/030294.
- International Written Opinion for International Patent application No. PCT/US2005/043951.
- International Search Report for International Patent application No. PCT/US2005/043951.
- Erdelyi et al. "Generation of diffraction-free beams for applications in optical microlithography", *J. Vac. Sci. Technol. B* 15 (12), Mar./Apr. 1997, pp. 287-292.
- International Search Report for International Patent application No. PCT/US2005/023664.
- International Written Opinion for International Patent application No. PCT/US2005/023664.
- Tearney et al., "Spectrally encoded miniature endoscopy" *Optical Society of America; Optical Letters* vol. 27, No. 6, Mar. 15, 2002; pp. 412-414.
- Yelin et al., "Double-clad Fiber for Endoscopy" *Optical Society of America; Optical Letters* vol. 29, No. 20, Oct. 16, 2005; pp. 2408-2410.
- International Search Report for International Patent application No. PCT/US2001/049704.
- International Search Report for International Patent application No. PCT/US2004/039454.
- International Written Opinion for International Patent application No. PCT/US2004/039454.
- Liptak David C. et al., (2007) "On the Development of a Confocal Rayleigh-Brillouin Microscope" *American Institute of Physics* vol. 78, 016106.
- Office Action mailed Oct. 1, 2008 for U.S. Appl. No. 11/955,986.
- Invitation of Pay Additional Fees mailed Aug. 7, 2008 for International Application No. PCT/US2008/062354.
- Invitation of Pay Additional Fees mailed Jul. 20, 2008 for International Application No. PCT/US2007/081982.
- International Search Report and Written Opinion mailed Mar. 7, 2006 for PCT/US2005/035711.
- International Search Report and Written Opinion mailed Jul. 18, 2008 for PCT/US2008/057533.
- Aizu, Y et al. (1991) "Bio-Speckle Phenomena and Their Application to the Evaluation of Blood Flow" *Optics and Laser Technology*, vol. 23, No. 4, Aug. 1, 1991.
- Richards G.J. et al. (1997) "Laser Speckle Contrast Analysis (LASCA): A Technique for Measuring Capillary Blood Flow Using the First Order Statistics of Laser Speckle Patterns" Apr. 2, 1997.
- Gonick, Maria M., et al (2002) "Visualization of Blood Microcirculation Parameters in Human Tissues by Time Integrated Dynamic Speckles Analysis" vol. 972, No. 1, Oct. 1, 2002.
- International Search Report and Written Opinion mailed Jul. 4, 2008 for PCT/US2008/051432.
- Jonathan, Enock (2005) "Dual Reference Arm Low-Coherence Interferometer-Based Reflectometer for Optical Coherence Tomography (OCT) Application" *Optics Communications* vol. 252.
- Motaghian Nezam, S.M.R. (2007) "increased Ranging Depth in optical Frequency Domain Imaging by Frequency Encoding" *Optics Letters*, vol. 32, No. 19, Oct. 1, 2007.
- Office Action dated Jun. 30, 2008 for U.S. Appl. No. 11/670,058.
- Office Action dated Jul. 7, 2008 for U.S. Appl. No. 10/551,735.
- Australian Examiner's Report mailed May 27, 2008 for Australian patent application No. 2003210669.
- Notice of Allowance mailed Jun. 4, 2008 for U.S. Appl. No. 11/174,425.
- European communication dated May 15, 2008 for European patent application No. 05819917.5.
- International Search Report and Written Opinion mailed Jun. 10, 2008 for PCT/US2008/051335.
- Oh, W.Y. et al (2006) "Ultra-high-Speed Optical Frequency Domain Imaging and Application to laser Ablation Monitoring" *Applied Physics Letters*, vol. 88.
- Office Action dated Aug. 21, 2008 for U.S. Appl. No. 11/505,700.
- Sticker, Markus (2002) *En Face Imaging of Single Cell layers by Differential Phase-Contrast Optical Coherence Microscopy* *Optics Letters*, col. 27, No. 13, Jul. 1, 2002.
- International Search Report and Written Opinion dated Jul. 17, 2008 for International Application No. PCT/US2008/057450.
- International Search Report and Written Opinion dated Aug. 11, 2008 for International Application No. PCT/US2008/058703.
- US National Library of Medicine (NLM), Bethesda, MD, US; Oct. 2007, "Abstracts of the 19th Annual Symposium of Transcatheter Cardiovascular Therapeutics, Oct. 20-25, 2007, Washington, DC, USA."
- International Search Report and Written Opinion dated May 26, 2008 for International Application No. PCT/US2008/051404.
- Office Action dated Aug. 25, 2008 for U.S. Appl. No. 11/264,655.
- Office Action dated Sep. 11, 2008 for U.S. Appl. No. 11/624,334.
- Office Action dated Aug. 21, 2008 for U.S. Appl. No. 11/956,079.
- Gelikono, V. M. et al. (Oct. 1, "Two-Wavelength Optical Coherence Tomography" *Radio physics and Quantum Electronics, Kluwer Academic Publishers-Consultants*. vol. 47, No. 10-1.
- International Search Report and Written Opinion for PCT/US2007/081982 dated Oct. 19, 2007.
- Database Compendex Engineering Information, Inc., New York, NY, US; Mar. 5, 2007, Yelin, Dvir et al: "Spectral-Domain Spectrally-Encoded Endoscopy".
- Database Biosis Biosciences Information Service, Philadelphia, PA, US; Oct. 2006, Yelin D. et al: "Three-Dimensional Miniature Endoscopy".
- International Search Report and Written Opinion mailed Mar. 14, 2005 for PCT/US2004/018045.

(56)

References Cited

OTHER PUBLICATIONS

Notification of the international Preliminary Report on Patentability mailed Oct. 21, 2005.

Shim M.G. et al., "Study of Fiber-Optic Probes for In vivo Medical Raman Spectroscopy" *Applied Spectroscopy*, vol. 53, No. 6, Jun. 1999.

Bingid U. et al., "Fibre-Optic Laser-Assisted Infrared Tumour Diagnostics (FLAIR); Infrared Tumour Diagnostics" *Journal of Physics D. Applied Physics*, vol. 38, No. 15, Aug. 7, 2005.

Jun Zhang et al. "Full Range Polarization-Sensitive Fourier Domain Optical Coherence Tomography" *Optics Express*, vol. 12, No. 24, Nov. 29, 2004.

Yonghua et al., "Real-Time Phase-Resolved Functional Optical Hilbert Transformation" *Optics Letters*, vol. 27, No. 2, Jan. 15, 2002.

Siavash et al., "Self-Referenced Doppler Optical Coherence Tomography" *Optics Letters*, vol. 27, No. 23, Dec. 1, 2002.

International Search Report and Written Opinion dated Dec. 20, 2004 for PCT/US04/10152.

Notification Concerning Transmittal of International Preliminary Report on Patentability dated Oct. 13, 2005 for PCT/US04/10152.

International Search Report and Written Opinion dated Mar. 23, 2006 for PCT/US2005/042408.

International Preliminary Report on Patentability dated Jun. 7, 2007 for PCT/US2005/042408.

International Search Report and Written Opinion dated Feb. 28, 2007 for International Application No. PCT/US2006/038277.

International Search Report and Written Opinion dated Jan. 30, 2009 for International Application No. PCT/US2008/081834.

International Search Report and Written Opinion dated Feb. 2, 2009 for International Application No. PCT/US2008/071786.

Bilenca A et al: "The Role of Amplitude and phase in Fluorescence Coherence Imaging: From Wide Filed to Nanometer Depth Profiling", *Optics IEEE*, May 5, 2007.

Inoue, Yusuke et al: "Variable Phase-Contrast Fluorescence Spectrometry for Fluorescently Strained Cells", *Applied Physics Letters*, Sep. 18, 2006.

Bernet, S et al: "Quantitative Imaging of Complex Samples by Spiral Phase Contrast Microscopy", *Optics Express*, May 9, 2006.

International Search Report and Written Opinion dated Jan. 15, 2009 for International Application No. PCT/US2008/074863.

Office Action dated Feb. 17, 2009 for U.S. Appl. No. 11/211,483.

Notice of Reasons for Rejection mailed Dec. 2, 2008 for Japanese patent application No. 2000-533782.

International Search Report and Written Opinion dated Feb. 24, 2009 for PCT/US2008/076447.

European Official Action dated Dec. 2, 2008 for EP 07718117.0.

Barfuss et al (1989) "Modified Optical Frequency Domain Reflectometry with High spatial Resolution for Components of integrated optic Systems", *Journal of Lightwave Technology*, IEEE vol. 7., No. 1.

Yun et al., (2004) "Removing the Depth-Degeneracy in Optical Frequency Domain Imaging with Frequency Shifting", *Optics Express*, vol. 12, No. 20.

International Search Report and Written Opinion dated Jun. 10, 2009 for PCT/US08/075456.

European Search Report issued May 5, 2009 for European Application No. 01991471.2.

Motz, J.T. et al: "Spectral- and Frequency-Encoded Fluorescence Imaging" *Optics Letters*, OSA, Optical Society of America, Washington, DC, US, vol. 30, No. 20, Oct. 15, 2005, pp. 2760-2762.

Japanese Notice of Reasons for Rejection dated Jul. 14, 2009 for Japanese Patent application No. 2006-503161.

Office Action dated Aug. 18, 2009 for U.S. Appl. No. 12/277,178.

Office Action dated Aug. 13, 2009 for U.S. Appl. No. 10/136,813.

Office Action dated Aug. 6, 2009 for U.S. Appl. No. 11/624,455.

Office Action dated May 15, 2009 for U.S. Appl. No. 11/537,123.

Office Action dated Apr. 17, 2009 for U.S. Appl. No. 11/537,343.

Office Action dated Apr. 15, 2009 for U.S. Appl. No. 12/205,775.

Office Action dated Dec. 9, 2008 for U.S. Appl. No. 09/709,162.

Office Action dated Dec. 23, 2008 for U.S. Appl. No. 11/780,261.

Office Action dated Jan. 9, 2010 for U.S. Appl. No. 11/624,455.

Office Action dated Feb. 18, 2009 for U.S. Appl. No. 11/285,301.

Beddow et al, (May 2002) "Improved Performance Interferometer Designs for Optical Coherence Tomography", *IEEE Optical Fiber Sensors Conference*, pp. 527-530.

Yaqoob et al., (Jun. 2002) "High-Speed Wavelength-Multiplexed Fiber-Optic Sensors for Biomedicine," *Sensors Proceedings of the IEEE*, pp. 325-330.

Office Action dated Feb. 18, 2009 for U.S. Appl. No. 11/697,012.

Zhang et al. (Sep. 2004), "Fourier Domain Functional Optical Coherence Tomography", *Saratov Fall Meeting 2004*, pp. 8-14.

Office Action dated Feb. 23, 2009 for U.S. Appl. No. 11/956,129.

Office Action dated Mar. 16, 2009 for U.S. Appl. No. 11/621,694.

Office Action dated Oct. 1, 2009 for U.S. Appl. No. 11/677,278.

Office Action dated Oct. 6, 2009 for U.S. Appl. No. 12/015,642.

Lin, Stollen et al., (1977) "A CW Tunable Near-infrared (1.085-1.175-um) Raman Oscillator," *Optics Letters*, vol. 1, 96.

Summons to attend Oral Proceedings dated Oct. 9, 2009 for European patent application No. 06813365.1.

Office Action dated Dec. 15, 2009 for U.S. Appl. No. 11/549,397.

R. Haggitt et al., "Barrett's Esophagus Correlation Between Mucin Histochemistry, Flow Cytometry, and Histological Diagnosis for Predicting increased Cancer Risk," *Apr. 1988, American Journal of Pathology*, vol. 131, No. 1, pp. 53-61.

R.H. Hardwick et al., (1995) "c-erbB-2 Overexpression in the Dysplasia/Carcinoma Sequence of Barrett's Oesophagus," *Journal of Clinical Pathology*, vol. 48, No. 2, pp. 129-132.

W. Polkowski et al, (1998) Clinical Decision making in Barrett's Oesophagus can be supported by Computerized Immunoquantitation and Morphometry of Features Associated with Proliferation and Differentiation, *Journal of pathology*, vol. 184, pp. 161-168.

J.R. Turner et al., MN Antigen Expression in Normal Preneoplastic, and Neoplastic Esophagus: A Clinicopathological Study of a New Cancer-Associated Biomarker, Jun. 1997, *Human Pathology*, vol. 28, No. 6, pp. 740-744.

D.J. Bowery et al. (1999) "Patterns of Gastritis in Patients with Gastro-Oesophageal Reflux Disease," *Gut*, vol. 45, pp. 798-803.

O'Reich et al., (2000) "Expression of Oestrogen and Progesterone Receptors in Low-Grade Endometrial Stromal Sarcomas," *British Journal of Cancer*, vol. 82, No. 5, pp. 1030-1034.

M.I. Canto et al., (1999) "Vital Staining and Barrett's Esophagus," *Gastrointestinal Endoscopy*, vol. 49, No. 3, Part 2, pp. S12-S16.

S. Jackle et al., (2000) "In Vivo Endoscopic Optical Coherence Tomography of the Human Gastrointestinal Tract-Toward Optical Biopsy," *Endoscopy*, vol. 32, No. 10, pp. 743-749.

E. Montgomery et al., "Reproducibility of the Diagnosis of Dysphasia in Barrett Esophagus: A Reaffirmation," *Apr. 2001, Human Pathology*, vol. 32, No. 4, pp. 368-378.

H. Geddert et al., "Expression of Cyclin B1 in the Metaplasia-Dysphasia-Carcinoma Sequence of Barrett Esophagus," *Jan. 2002, Cancer*, vol. 94, No. 1, pp. 212-218.

P. Pfau et al., (2003) "Criteria for the Diagnosis of Dysphasia by Endoscopic Optical Coherence Tomography," *Gastrointestinal Endoscopy*, vol. 58, No. 2, pp. 196-2002.

R. Kiesslich et al., (2004) "Confocal Laser Endoscopy for Diagnosing Intraepithelial Neoplasias and Colorectal Cancer in Vivo," *Gastroenterology*, vol. 127, No. 3, pp. 706-713.

X. Qi et al., (2004) "Computer Aided Diagnosis of Dysphasia in Barrett's Esophagus Using Endoscopic Optical Coherence Tomography," *SPIE, Coherence Domain Optical Methods and Conference Tomography in Biomedicine VIII. Proc. of Conference on*, vol. 5316, pp. 33-40.

Seltzer et al., (1991) "160 nm Continuous Tuning of a MQW Laser in an External Cavity Across the Entire 1.3 um Communications Window," *Electronics Letters*, vol. 27, pp. 95-96.

Office Action dated Jan. 25, 2010 for U.S. Appl. No. 11/537,048.

International Search Report dated Jan. 27, 2010 for PCT/US2009/050553.

International Search Report dated Jan. 27, 2010 for PCT/US2009/047988.

International Search Report dated Feb. 23, 2010 for U.S. Appl. No. 11/445,131.

Office Action dated Mar. 18, 2010 of U.S. Appl. No. 11/844,454.

(56)

References Cited

OTHER PUBLICATIONS

- Office Action dated Apr. 8, 2010 of U.S. Appl. No. 11/414,564.
- Japanese Office Action dated Apr. 13, 2010 for Japanese Patent application No. 2007-515029.
- International Search Report dated May 27, 2010 for PCT/US2009/063420.
- Office Action dated May 28, 2010 for U.S. Appl. No. 12/015,642.
- Office Action dated Jun. 2, 2010 for U.S. Appl. No. 12/112,205.
- Office Action dated Jul. 7, 2010 for U.S. Appl. No. 11/624,277.
- Montag Ethan D., "Parts of the Eye" online textbook for JIMG 774: Vision & Pscophysics, download on Jun. 23, 2010 from http://www.cis.rit.edu/people/faculty/montag/vandplite/pages/chap_8/ch8p3.html.
- Office Action dated Jul. 16, 2010 for U.S. Appl. No. 11/445,990.
- Office Action dated Jul. 20, 2010 for U.S. Appl. No. 11/625,135.
- Office Action dated Aug. 5, 2010 for U.S. Appl. No. 11/623,852.
- Chinese office action dated Aug. 4, 2010 for CN 200780005949.9.
- Chinese office action dated Aug. 4, 2010 for CN 200780016266.3.
- Zhang et al., "Full Range Polarization-Sensitive Fourier Domain Optical Coherence Tomography" *Optics Express*, Nov. 29, 2004, vol. 12, No. 24.
- Office Action dated Aug. 27, 2010 for U.S. Appl. No. 11/569,790.
- Office Action dated Aug. 31, 2010 for U.S. Appl. No. 11/677,278.
- Office Action dated Sep. 3, 2010 for U.S. Appl. No. 12/139,314.
- Yong Zhao et al: "Virtual Data Grid Middleware Services for Data-Intensive Science", *Concurrency and Computation: Practice and Experience*, Wiley, London, GB, Jan. 1, 2000, pp. 1-7, pp. 1532-0626.
- Swan et al., "Toward Nanometer-Scale Resolution in Fluorescence Microscopy using Spectral Self-Interference" *IEEE Journal. Selected Topics in Quantum Electronics* 9 (2) 2003, pp. 294-300.
- Moiseev et al., "Spectral Self-Interference Fluorescence Microscopy", *J. Appl. Phys.* 96 (9) 2004, pp. 5311-5315.
- Hendrik Verschueren, "Interference Reflection Microscopy in Cell Biology", *J. Cell Sci.* 75, 1985, pp. 289-301.
- Park et al., "Diffraction Phase and Fluorescence Microscopy", *Opt. Expr.* 14 (18) 2006, pp. 8263-8268.
- Swan et al., "High Resolution Spectral Self-Interference Fluorescence Microscopy", *Proc. SPIE* 4621, 2002, pp. 77-85.
- Sanchez et al., "Near-Field Fluorescence Microscopy Based on Two-Photon Excitation with Metal Tips", *Phys. Rev. Lett.* 82 (20) 1999, pp. 4014-4017.
- Wojtkowski, Maciej, Ph.D. "Three-Dimensional Retinal Imaging with High-Speed Ultrahigh-Resolution Optical Coherence Tomography" *Ophthalmology*, Oct. 2005, 112(10): 1734-1746.
- Vaughan, J.M. et al., "Brillouin Scattering, Density and Elastic Properties of the Lens and Cornea of the Eye", *Nature*, vol. 284, Apr. 3, 1980, pp. 489-491.
- Hess, S.T. et al. "Ultra-high Resolution Imaging by Fluorescence Photoactivation Localization Microscopy" *Biophysical Journal* vol. 91, Dec. 2006, 4258-4272.
- Fernandez-Suarez, M. et al., "Fluorescent Probes for Super-Resolution Imaging in Living Cells" *Nature Reviews Molecular Cell Biology* vol. 9, Dec. 2008.
- Extended European Search Report mailed Dec. 14, 2010 for EP 10182301.1.
- S. Hell et al., "Breaking the diffraction resolution limit by stimulated-emission—stimulated-emission-depletion fluorescence microscopy," *Optics Letters*. 19:495 (1995) and *Ground State Depletion (GSD)*.
- S. Hell et al. "Ground-State-Depletion fluorescence microscopy—a concept for breaking the diffraction resolution limit," *Applied Physics B*. 60:780 (1994) fluorescence microscopy, photo-activated localization microscopy (PALM).
- E. Betzig et al. "Imaging intracellular fluorescent proteins at nanometer resolution," *Science* 313:1642 (2006), stochastic optical reconstruction microscopy (STORM).
- M. Rust et al. "Sub-diffraction-limited imaging by stochastic optical reconstruction microscopy (STORM)," *Nature Methods* 3:783 (2006), and structured illumination microscopy (SIM).
- B. Bailey et al. "Enhancement of Axial Resolution in Fluorescence Microscopy by Standing-Wave Excitation," *Nature* 366:44 (1993).
- M. Gustafsson "Surpassing the lateral resolution limit by a factor of two using structured illumination microscopy," *Journal of Microscopy* 198:82 (2000).
- M. Gustafsson "Nonlinear structured illumination microscopy: Wide-field fluorescence imaging with theoretically unlimited resolution," *PNAS* 102:13081 (2005).
- R. Thompson et al. "Precise nanometer localization analysis for individual fluorescent probes," *Biophysical Journal* 82:2775 (2002).
- K. Drabe et al. "Localization of Spontaneous Emission in front of a mirror," *Optics Communications* 73:91 (1989).
- Swan et al. "Toward nanometer-scale resolution in fluorescence microscopy using spectral self-interference," *IEEE Quantum Electronics* 9:294 (2003).
- C. Joo, et al. "Spectral Domain optical coherence phase and multiphoton microscopy," *Optics Letters* 32:623 (2007).
- Virmani et al., "Lesions from sudden coronary death: A comprehensive morphological classification scheme for atherosclerotic lesions," *Arterioscler. Thromb. Vase. Bio.*, 20:1262-75 (2000).
- Gonzalez, R.C. and Wintz, P., "Digital Image Processing" Addison-Wesley Publishing Company, Reading MA, 1987.
- V. Tuchin et al., "Speckle interferometry in the measurements of tissues vibrations," *SPIE*, 1647: 125 (1992).
- A.A. Bednov et al., "Investigation of Statistical Properties of Lymph Flow Dynamics Using Speckle-Microscopy," *SPIE*, 2981: 181-90 (1997).
- Feng et al., "Mesoscopic Conductors and Correlations in Laser Speckle Patterns" *Science, New Series*, vol. 251, No. 4994, pp. 633-639 (Feb. 8, 1991).
- Lee et al., "The Unstable Atheroma," *Arteriosclerosis, Thrombosis & Vascular Biology*, 17:1859-67 (1997).
- International Search report dated Apr. 29, 2011 for PCT/US2010/051715.
- International Search report dated Sep. 13, 2010 for PCT/US2010/023215.
- International Search Report dated Jul. 28, 2011 for PCT/US2010/059534.
- International Search report dated Nov. 18, 2011 for PCT/US2011/027450.
- International Search report dated Nov. 18, 2011 for PCT/US2011/027437.
- International Search report dated Nov. 22, 2011 for PCT/US2011/027421.
- Poneros et al: "Optical Coherence Tomography of the Biliary Tree During ERCP", *Gastrointestinal Endoscopy*, Elsevier, NL, vol. 55, No. 1, Jan. 1, 2002, pp. 84-88.
- Fu L et al: double-Clad Photonic Crystal Fiber Coupler for compact Nonlinear Optical Microscopy Imaging, *Optics Letters*, OSA, Optical Society of America, vol. 31, No. 10, May 15, 2006, pp. 1471-1473.
- Japanese language Appeal Decision dated Jan. 10, 2012 for JP 2006-503161.
- Japanese Notice of Grounds for Rejection dated Oct. 28, 2011 for JP2009-294737.
- Japanese Notice of Grounds for Rejection dated Dec. 28, 2011 for JP2008-535793.
- Japanese Notice of Reasons for Rejection dated Dec. 12, 2011 for JP 2008-533712.
- International Search Report and Written Opinion mailed Feb. 9, 2012 based on PCT/US2011/034810.
- Japanese Notice of Reasons for Rejection dated Mar. 27, 2012 for JP 2003-102672.
- Japanese Notice of Reasons for Rejection dated May 8, 2012 for JP 2008-533727.
- Korean Office Action dated May 25, 2012 for KR 10-2007-7008116.
- Japanese Notice of Reasons for Rejection dated May 21, 2012 for JP 2008-551523.
- Japanese Notice of Reasons for Rejection dated Jun. 20, 2012 for JP 2009-546534.
- European Official Communication dated Aug. 1, 2012 for EP 10193526.0.
- European Search Report dated Jun. 25, 2012 for EP 10733985.5.

(56)

References Cited

OTHER PUBLICATIONS

Wieser, Wolfgang et al., "Multi-Megahertz OCT: High Quality 3D Imaging at 20 million A-Scans and 4.5 Gvoxels Per Second" Jul. 5, 2010, vol. 18, No. 14, Optics Express.

European Communication Pursuant to EPC Article 94(3) for EP 07845206.7 dated Aug. 30, 2012.

International Search Report and Written Opinion mailed Aug. 30, 2012 for PCT/US2012/035234.

Giuliano, Scarcelli et al., "Three-Dimensional Brillouin Confocal Microscopy". Optical Society of American, 2007, CtuV5.

Giuliano, Scarcelli et al., "Confocal Brillouin Microscopy for Three-Dimensional Mechanical Imaging." Nat Photonics, Dec. 9, 2007.

Japanese Notice of Reasons for Rejections dated Oct. 10, 2012 for 2008-553511.

W.Y. Oh et al: "High-Speed polarization Sensitive optical Frequency Domain Imaging with Frequency Multiplexing", Optics Express, vol. 16, No. 2, Jan. 1, 2008.

Athey, B.D. et al., "Development and Demonstration of a Networked Telepathology 3-D Imaging, Databasing, and Communication System", 1998 ("C2"), pp. 5-17.

D'Amico, A.V., et al., "Optical Coherence Tomography as a Method for Identifying Benign and Malignant Microscopic Structures in the Prostate Gland", Urology, vol. 55, Issue 5, May 2000 ("C3"), pp. 783-787.

Tearney, G.J. et al., "In Vivo Endoscopic Optical Biopsy with Optical Coherence Tomography", Science, vol. 276, No. 5321, Jun. 27, 1997 ("C6"), pp. 2037-2039.

Japanese Notice of Reasons for Rejections dated Oct. 2, 2012 for 2007-543626.

Canadian Office Action dated Oct. 10, 2012 for 2,514,189.

Japanese Notice of Reasons for Rejections dated Nov. 9, 2012 for JP 2007-530134.

Japanese Notice of Reasons for Rejections dated Nov. 27, 2012 for JP 2009-554772.

Japanese Notice of Reasons for Rejections dated Oct. 11, 2012 for JP 2008-533712.

Yoden, K. et al. "An Approach to Optical Reflection Tomography Along the Geometrical Thickness," Optical Review, vol. 7, No. 5, Oct. 1, 2000.

International Search Report and Written Opinion mailed Oct. 25, 2012 for PCT/US2012/047415.

Joshua, Fox et al: "Measuring Primate RNFL Thickness with OCT", IEEE Journal of Selected Topics in Quantum Electronics, IEEE Service Center, Piscataway, NJ, US, vol. 7, No. 6, Nov. 1, 2001.

European Official Communication dated Feb. 6, 2013 for 04822169.1.

International Search Report mailed Jan. 31, 2013 for PCT/US2012/061135.

Viliyam K. Pratt. Lazernye Sistemy Svyazi. Moskva, Izdatelstvo "Svyaz", 1972. p. 68-70.

International Search Report and Written Opinion mailed Jan. 31, 2013 for PCT/US2012/060843.

European Search Report mailed on Mar. 11, 2013 for EP 10739129.4.

Huber, R. et al: "Fourier Domain Mode Locked Lasers for OCT Imaging at up to 290 kHz Sweep Rates", Proceedings of SPIE, SPIE—International Society for Optical Engineering, US, vol. 5861, No. 1, Jan. 1, 2005.

M. Kourogi et al: "Programmable High Speed (1MHz) Vernier-mode-locked Frequency-Swept Laser for OCT Imaging", Proceedings of SPIE, vol. 6847, Feb. 7, 2008.

Notice of Reasons for Rejection dated Feb. 5, 2013 for JP 2008-509233.

Notice of Reasons for Rejection dated Feb. 19, 2013 for JP 2008-507983.

European Extended Search Report mailed Mar. 26, 2013 for EP 09825421.1.

Masahiro, Yamanari et al: "polarization-Sensitive Swept-Source Optical Coherence Tomography with Continuous Source Polarization Modulation", Optics Express, vol. 16, No. 8, Apr. 14, 2008.

European Extended Search Report mailed on Feb. 1, 2013 for EP 12171521.3.

Nakamura, Koichiro et al., "A New Technique of Optical Ranging by a Frequency-Shifted Feedback Laser", IEEE Photonics Technology Letters, vol. 10, No. 12, pp. 1041-1135, Dec. 1998.

Lee, Seok-Jeong et al., "Ultrahigh Scanning Speed Optical Coherence Tomography Using Optical Frequency Comb Generators", The Japan Society of Applied Physics, vol. 40 (2001).

Kinoshita, Masaya et al., "Optical Frequency-Domain Imaging Microprofilometry with a Frequency-Tunable Liquid-Crystal Fabry-Perot Etalon Device" Applied Optics, vol. 38, No. 34, Dec. 1, 1999.

Japanese Notice of Reasons for Rejection mailed Apr. 16, 2013 for JP 2009-510092.

Bachmann A.H. et al: "Heterodyne Fourier Domain Optical Coherence Tomography for Full Range Probing with High Axial Resolution", Optics Express, OSA, vol. 14, No. 4, Feb. 20, 2006.

European Search Report for 12194876.4 dated Feb. 1, 2013.

First Office Action for Japanese Patent Application No. 2014-108477 mailed on Mar. 3, 2015.

* cited by examiner

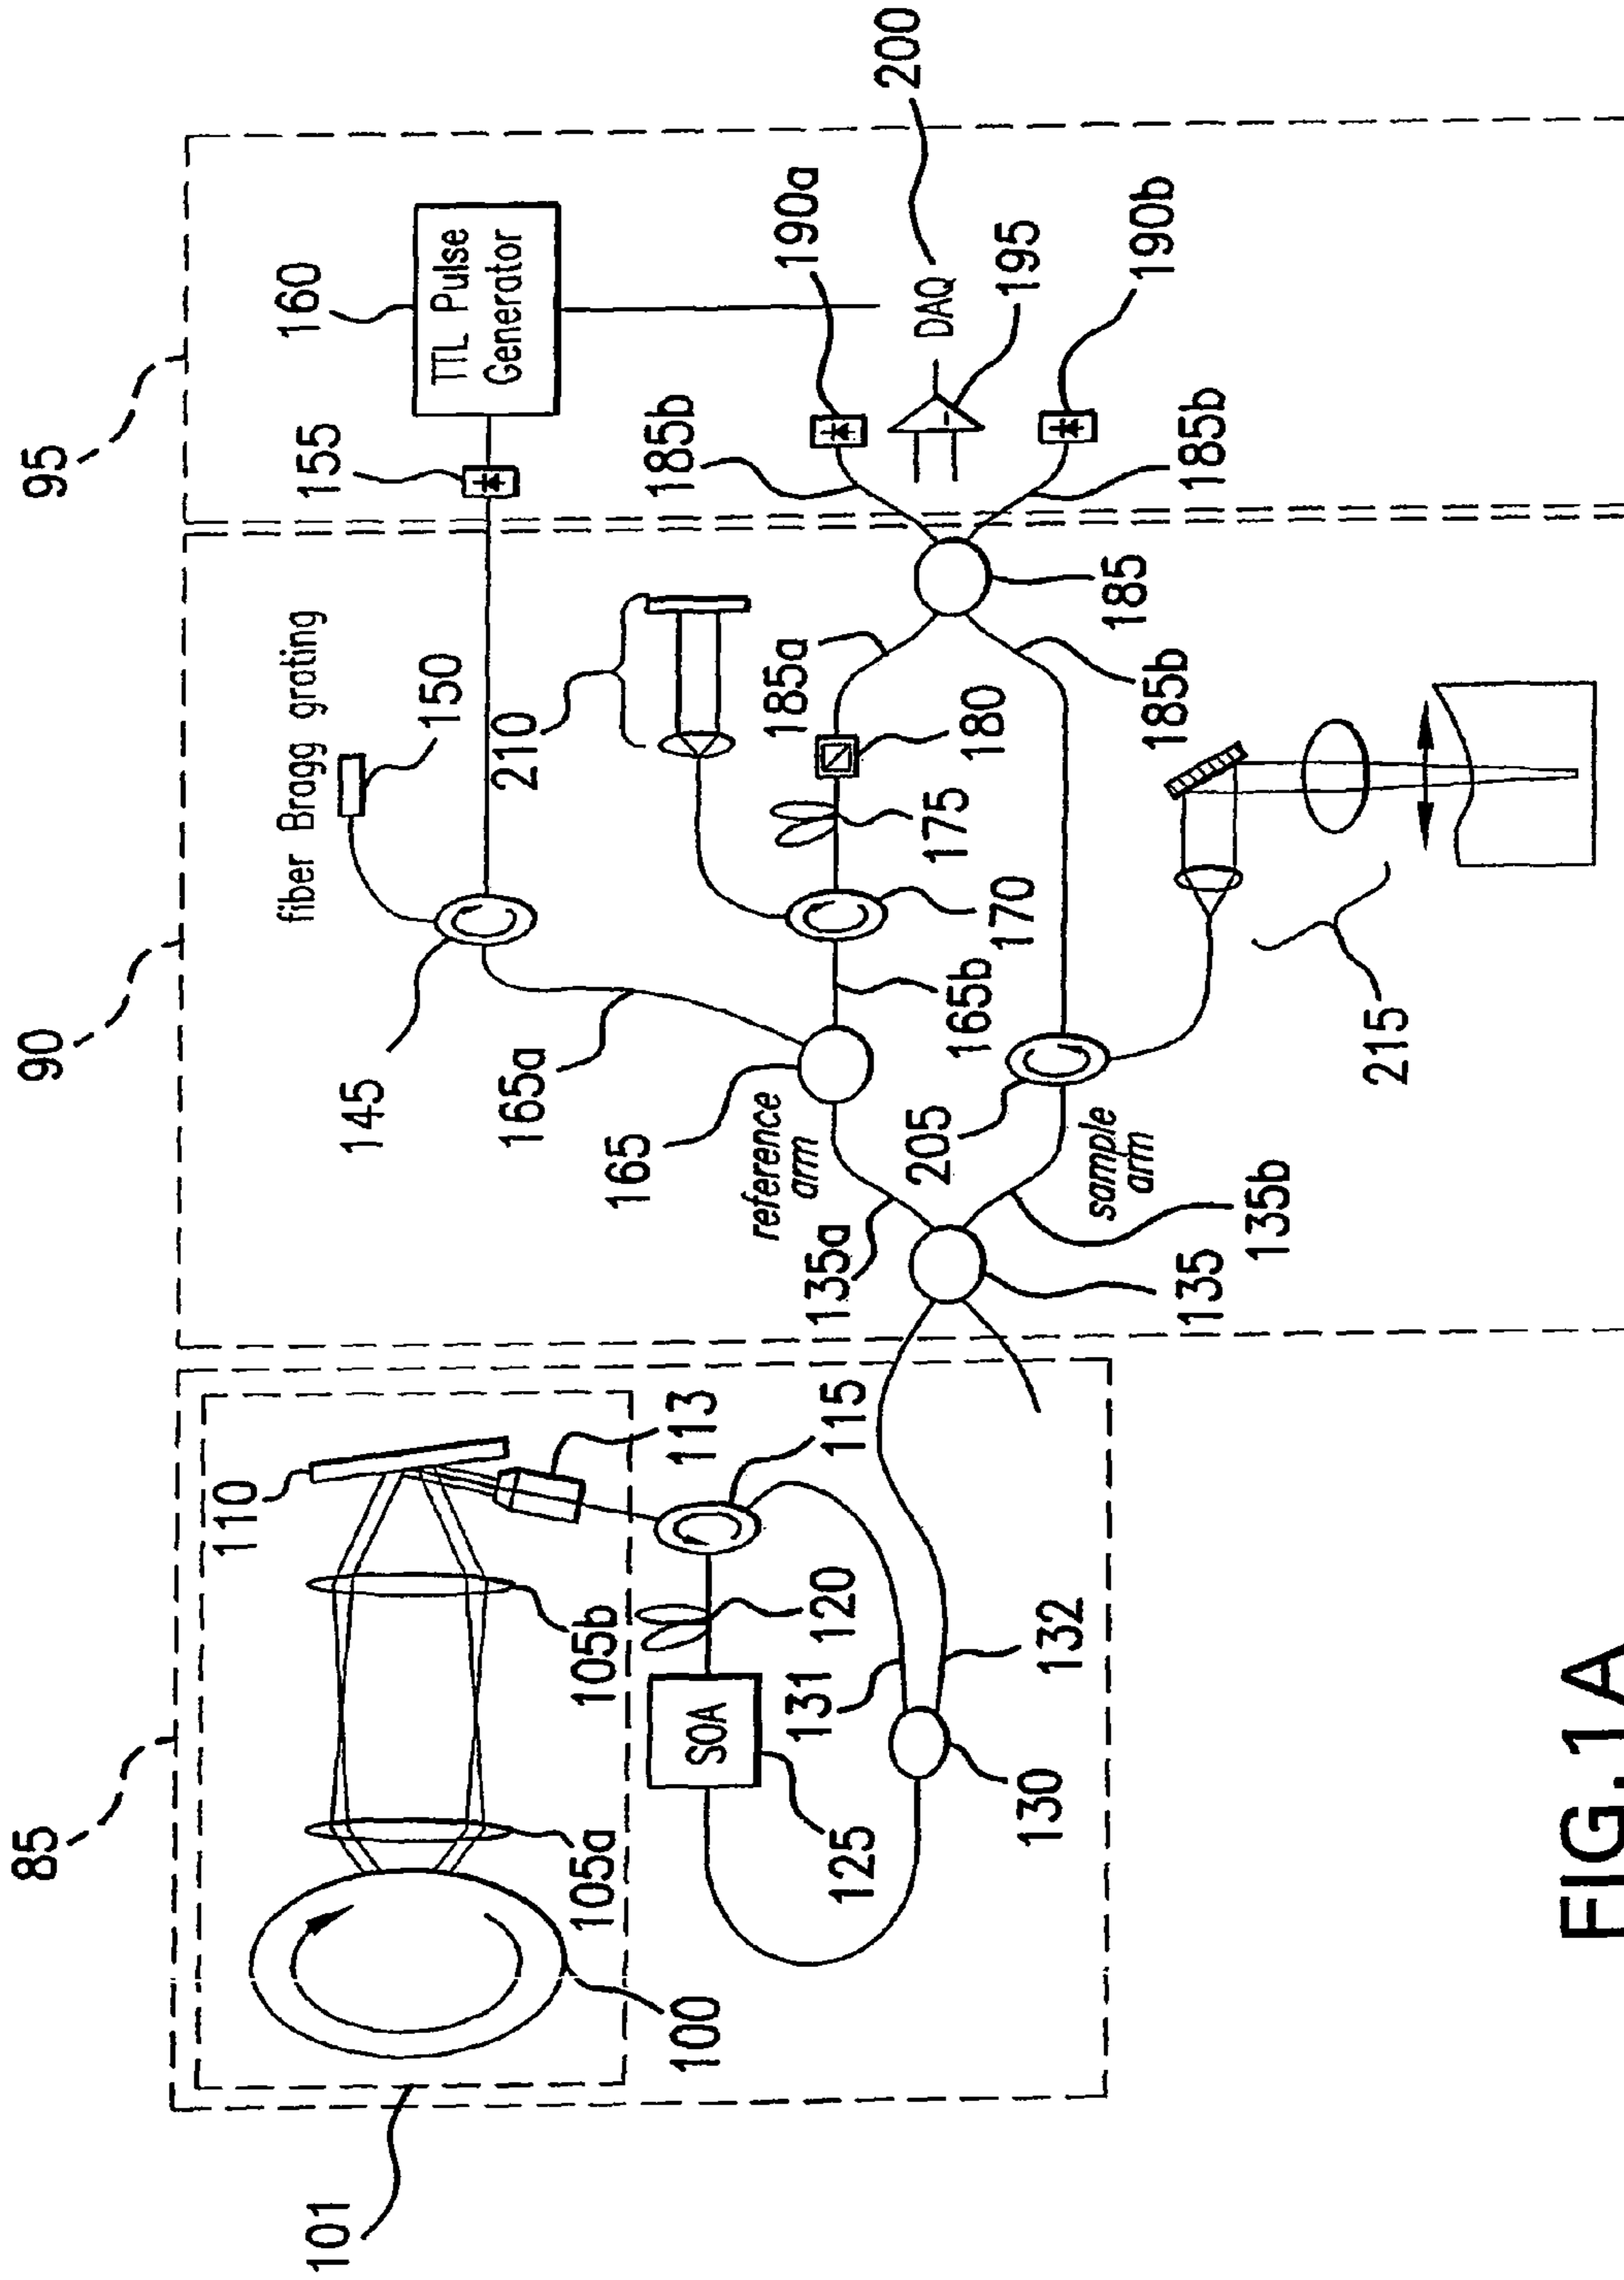


FIG. 1A

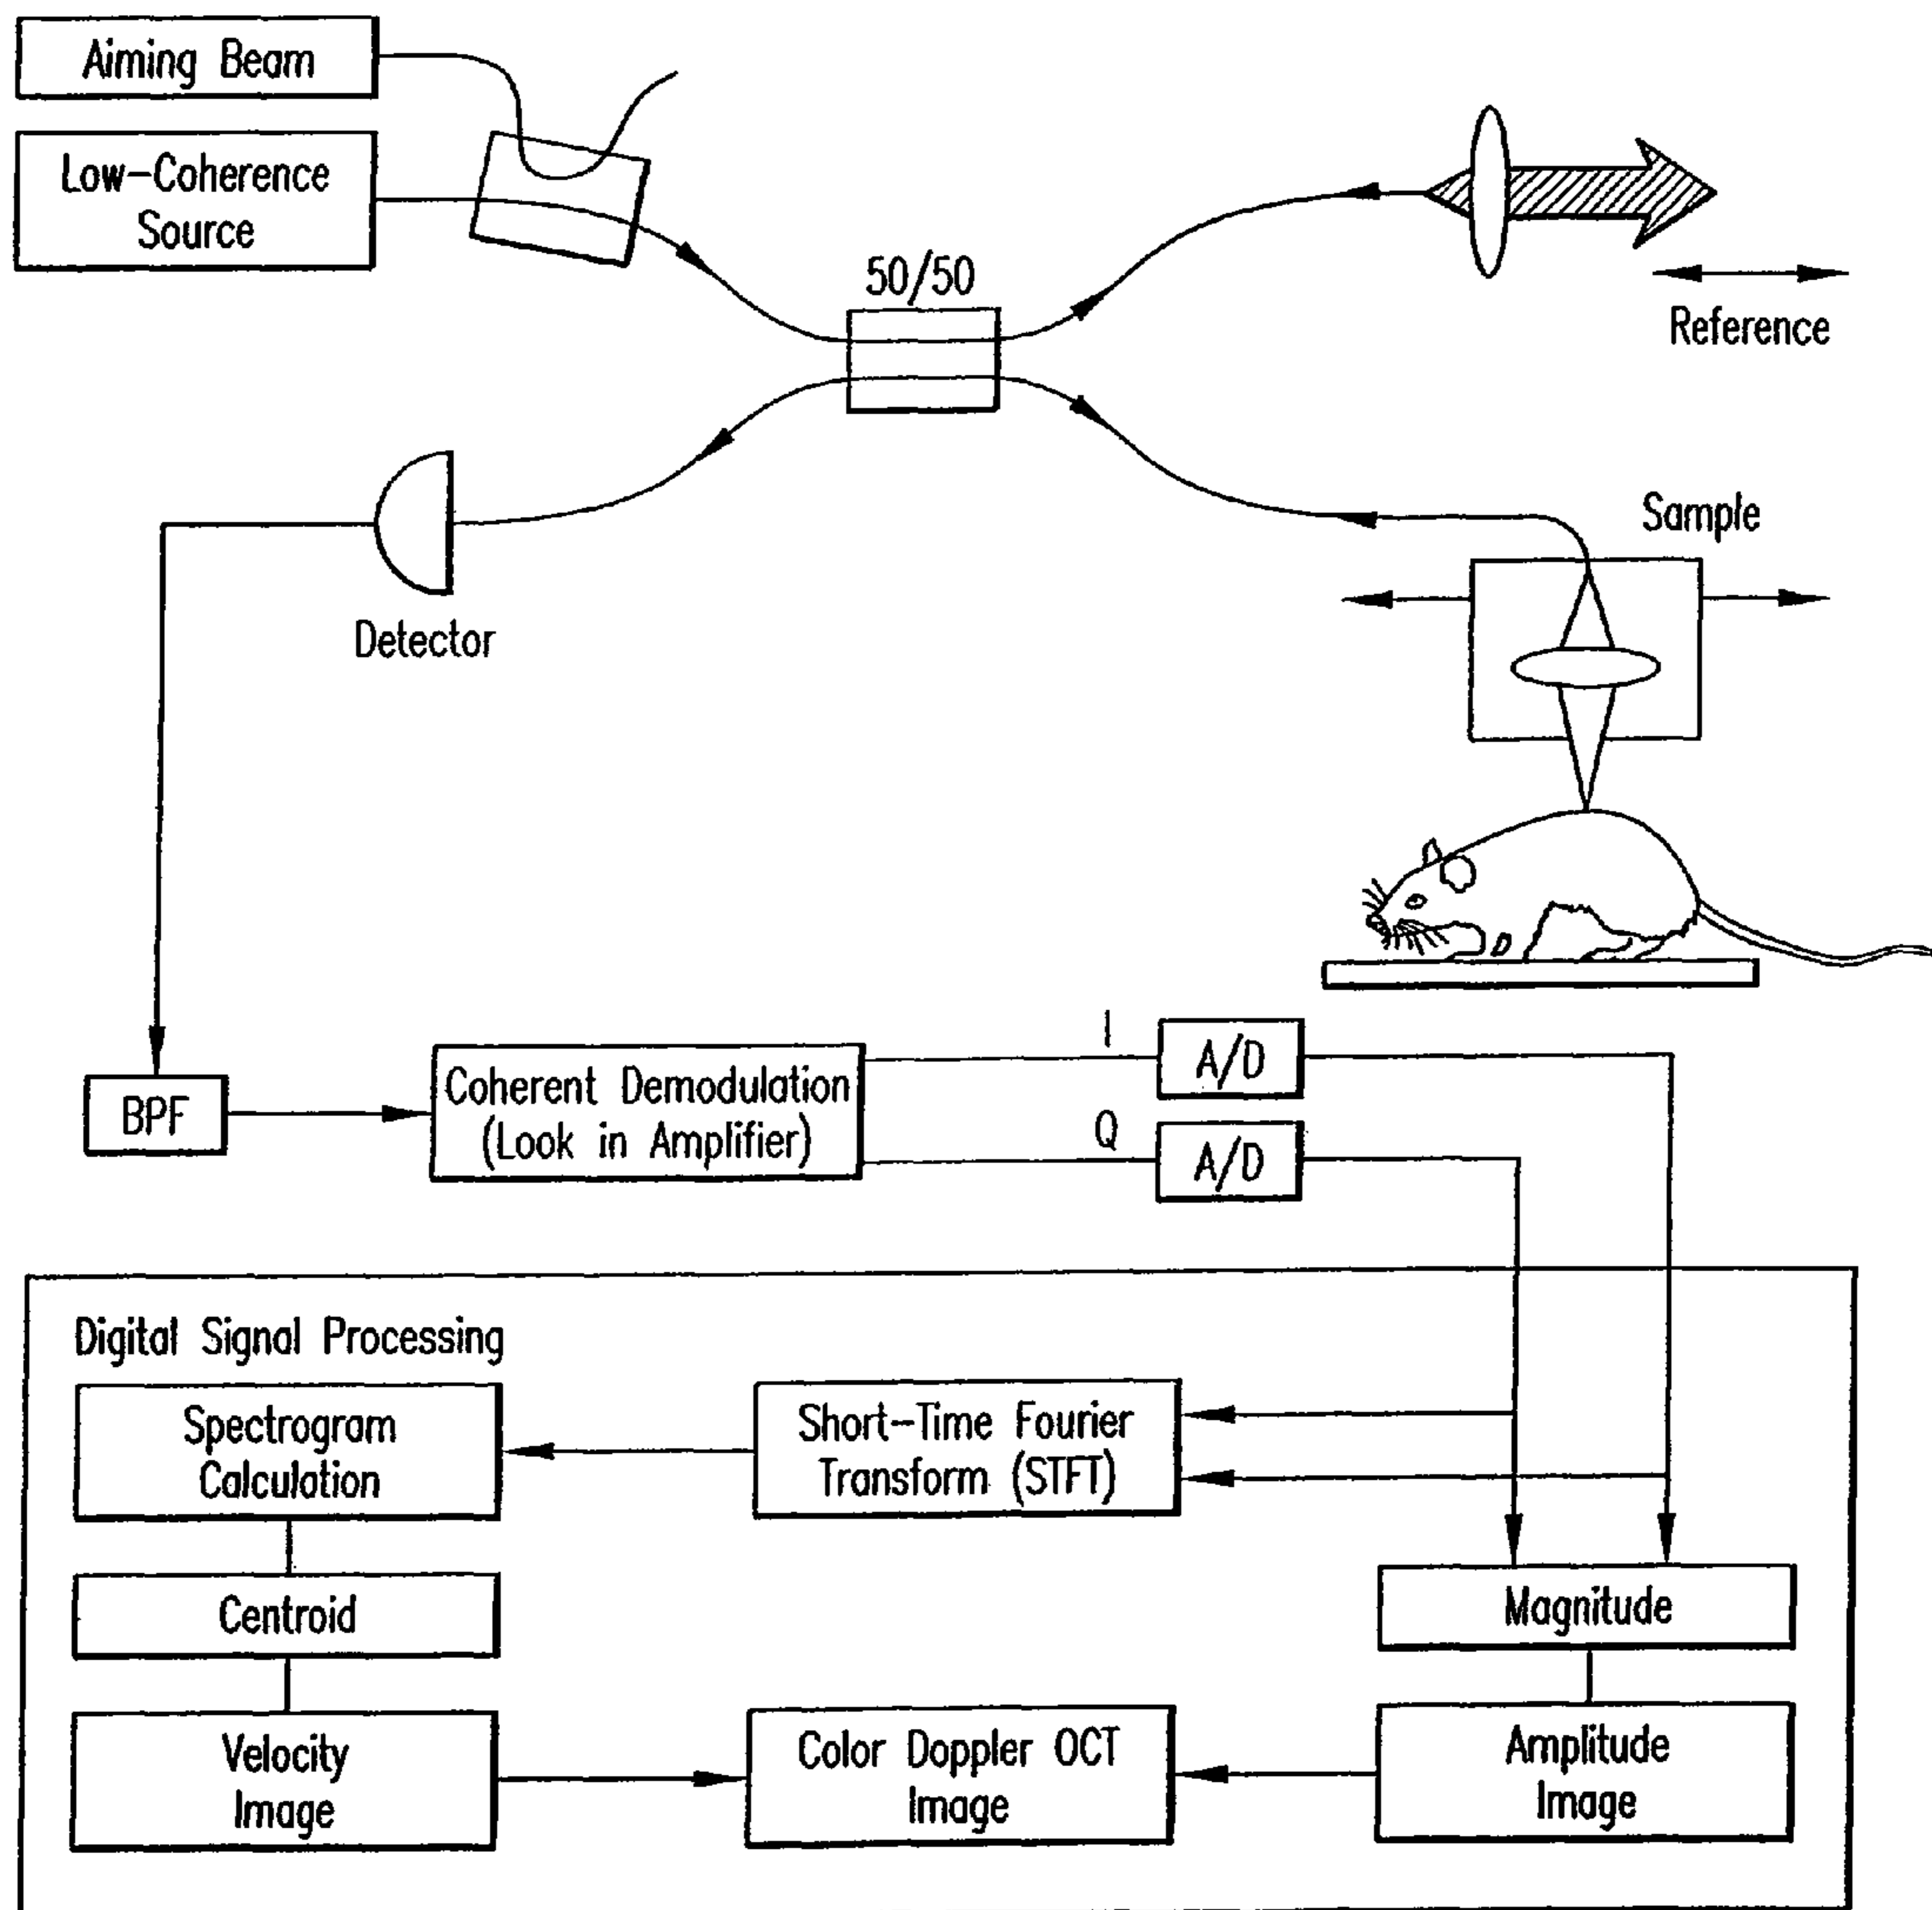


FIG. 1B

PRIOR ART

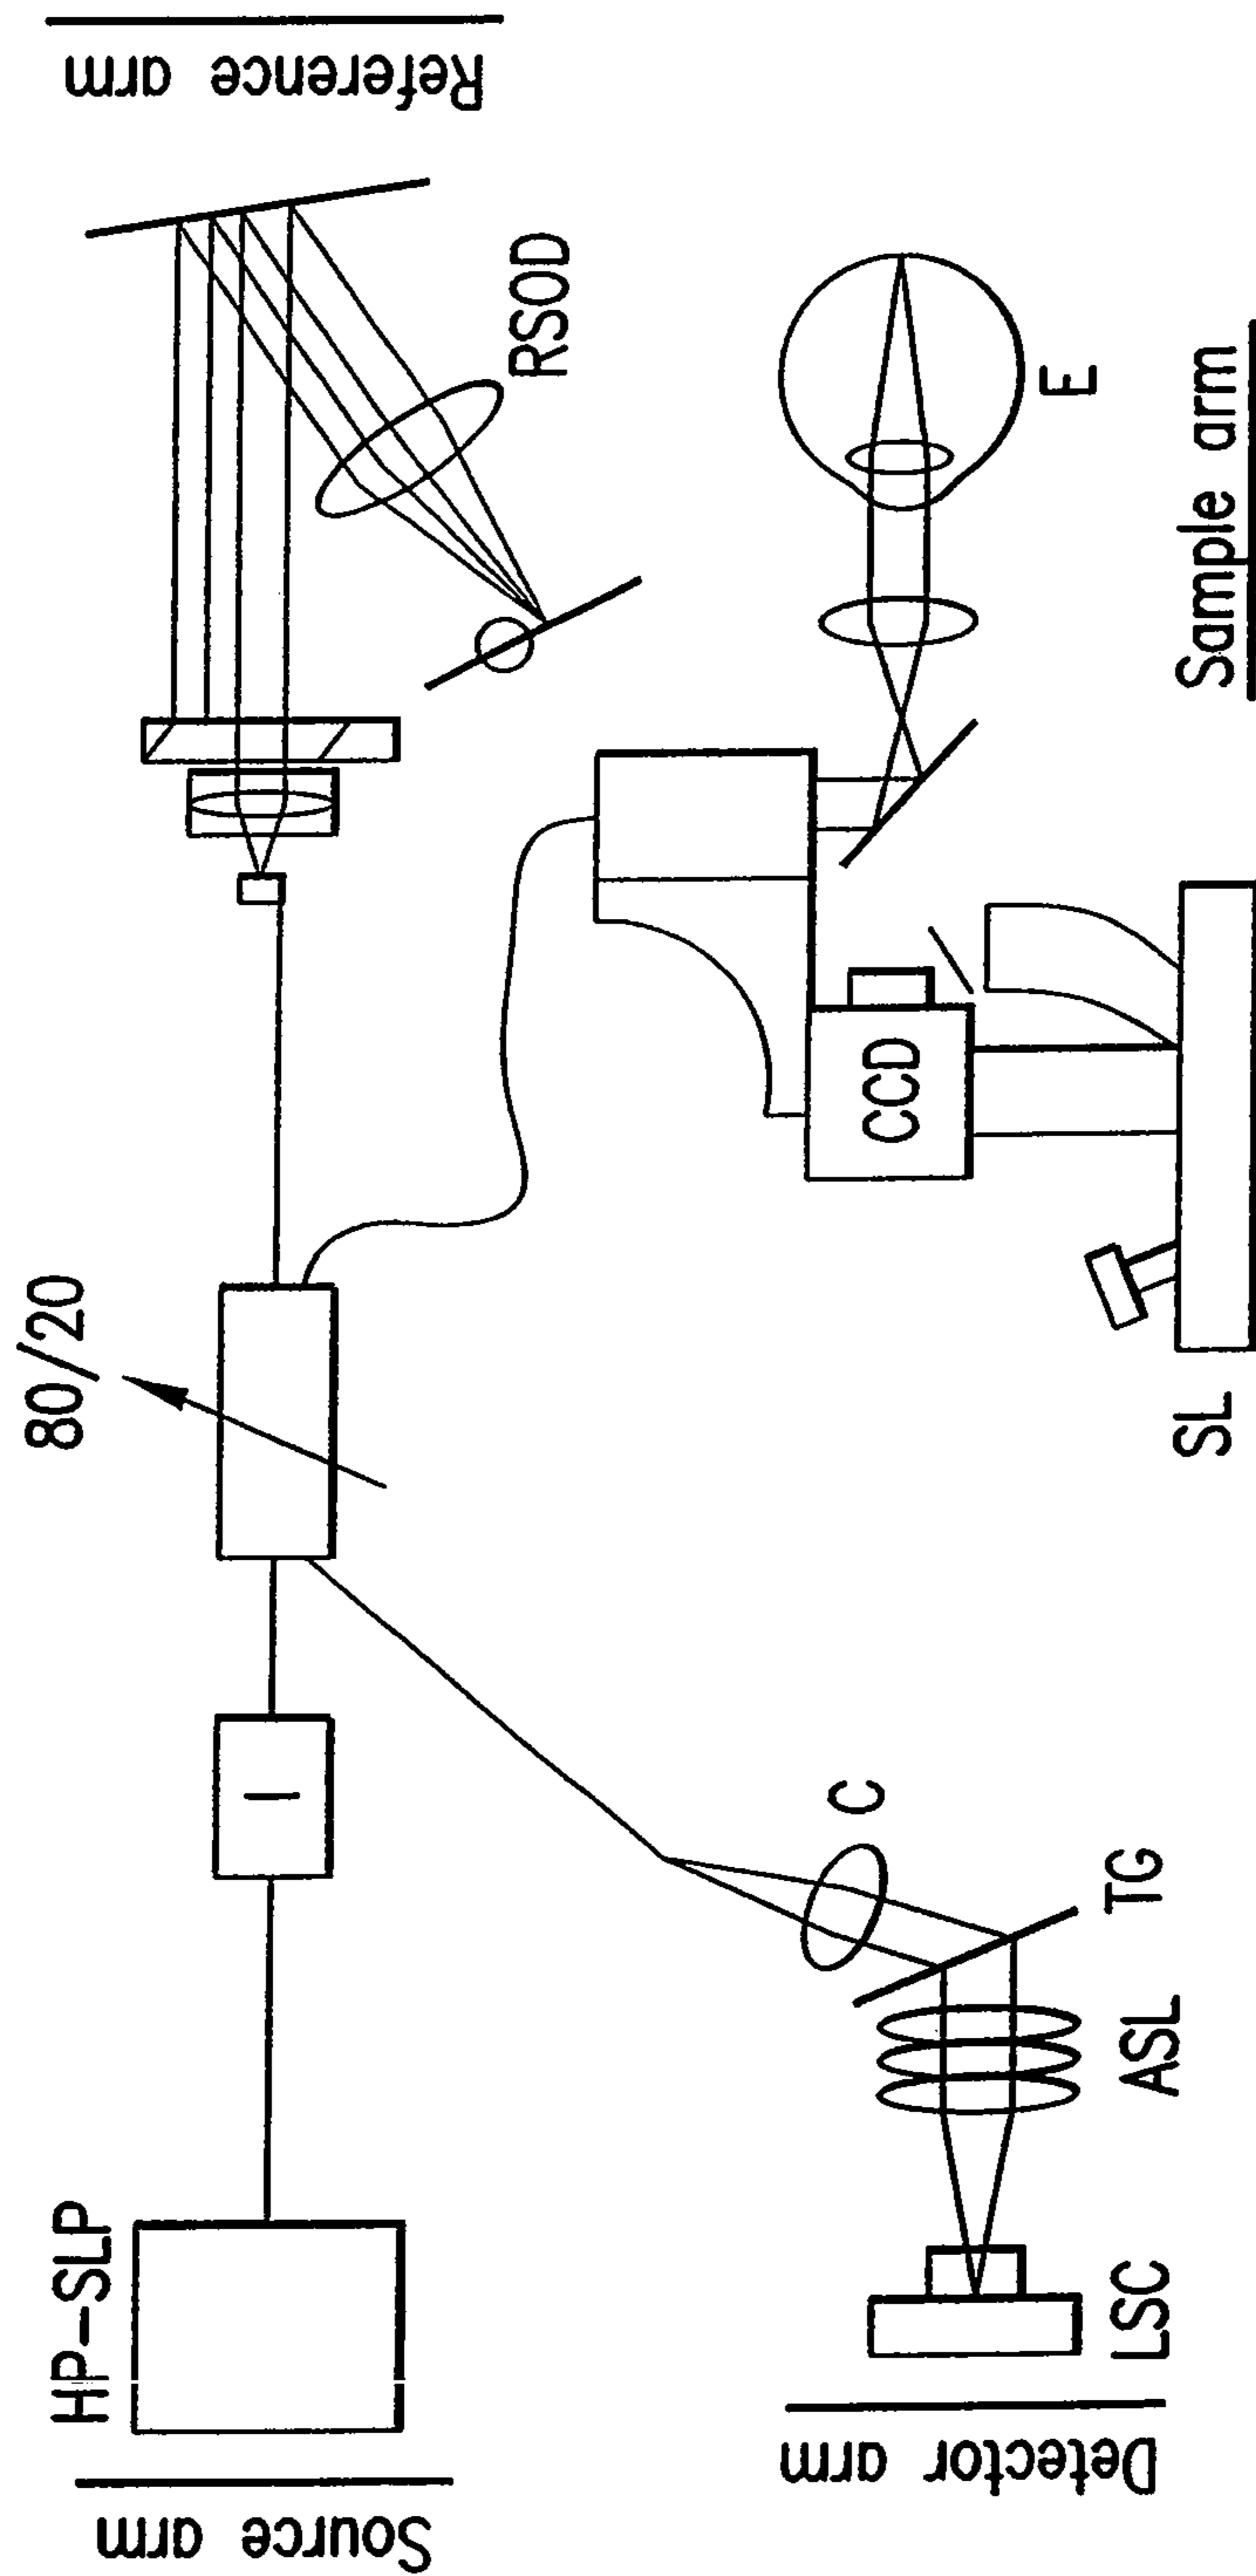


FIG.1C

PRIOR ART

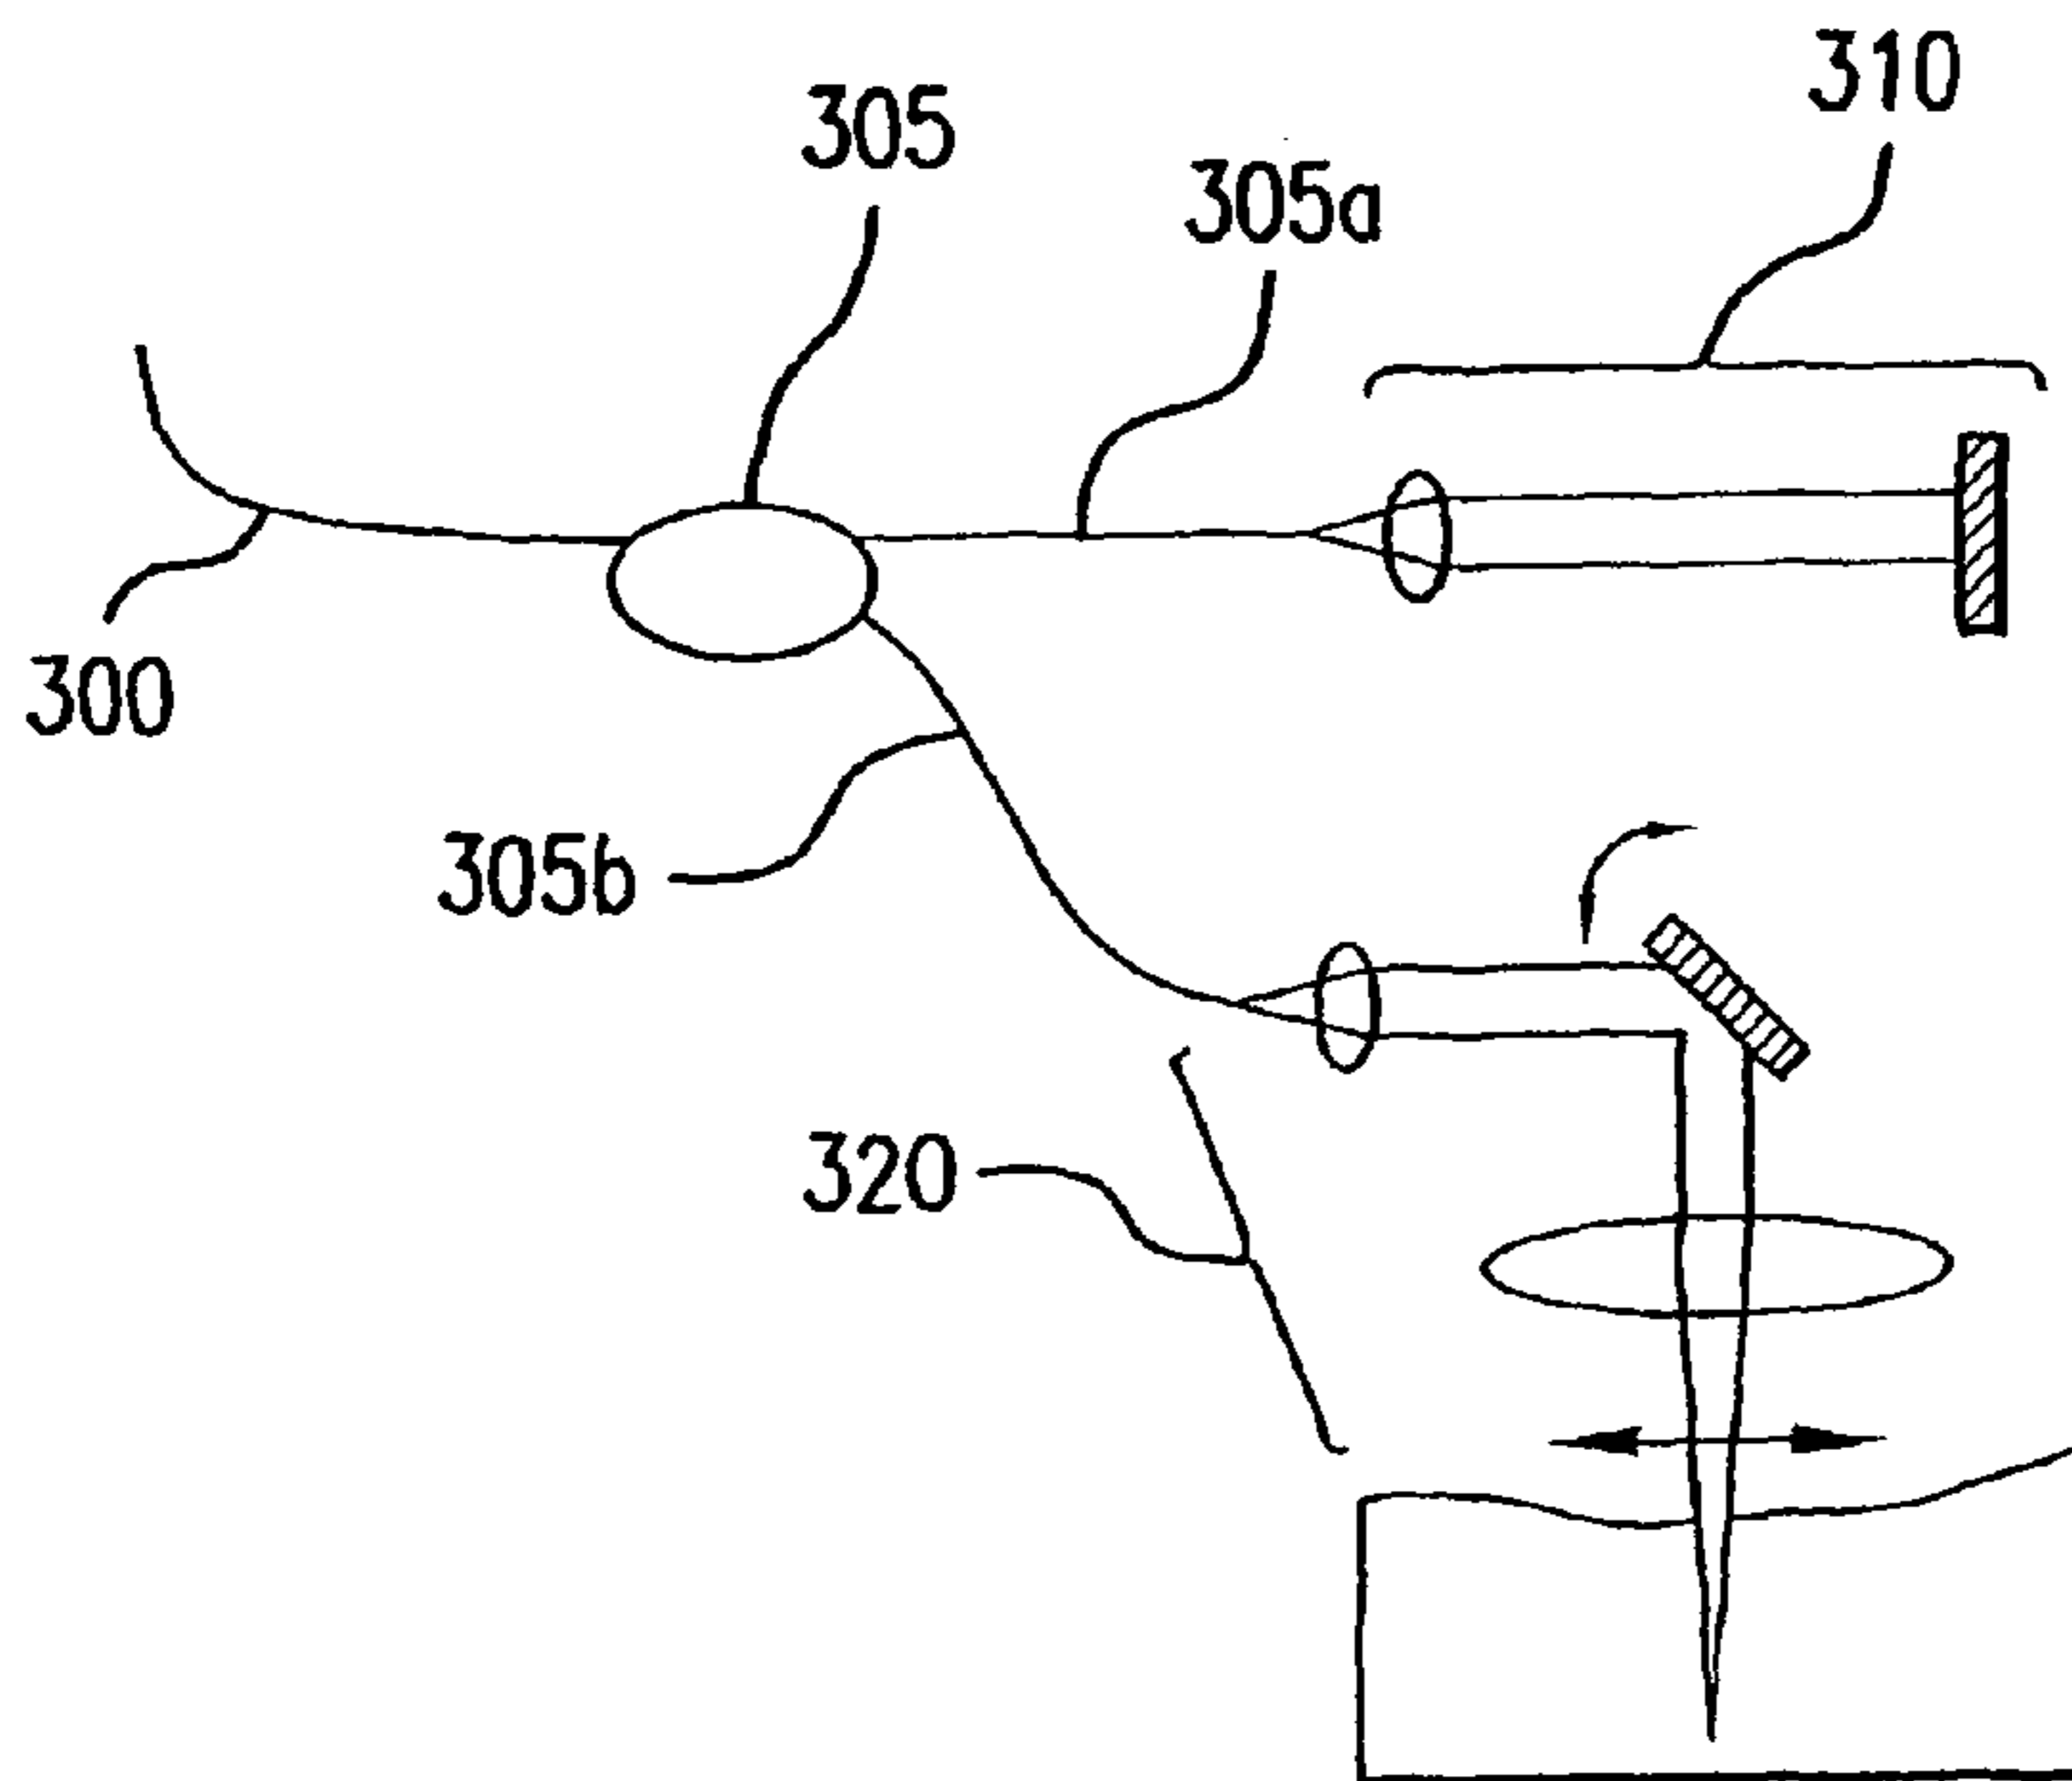


FIG. 2

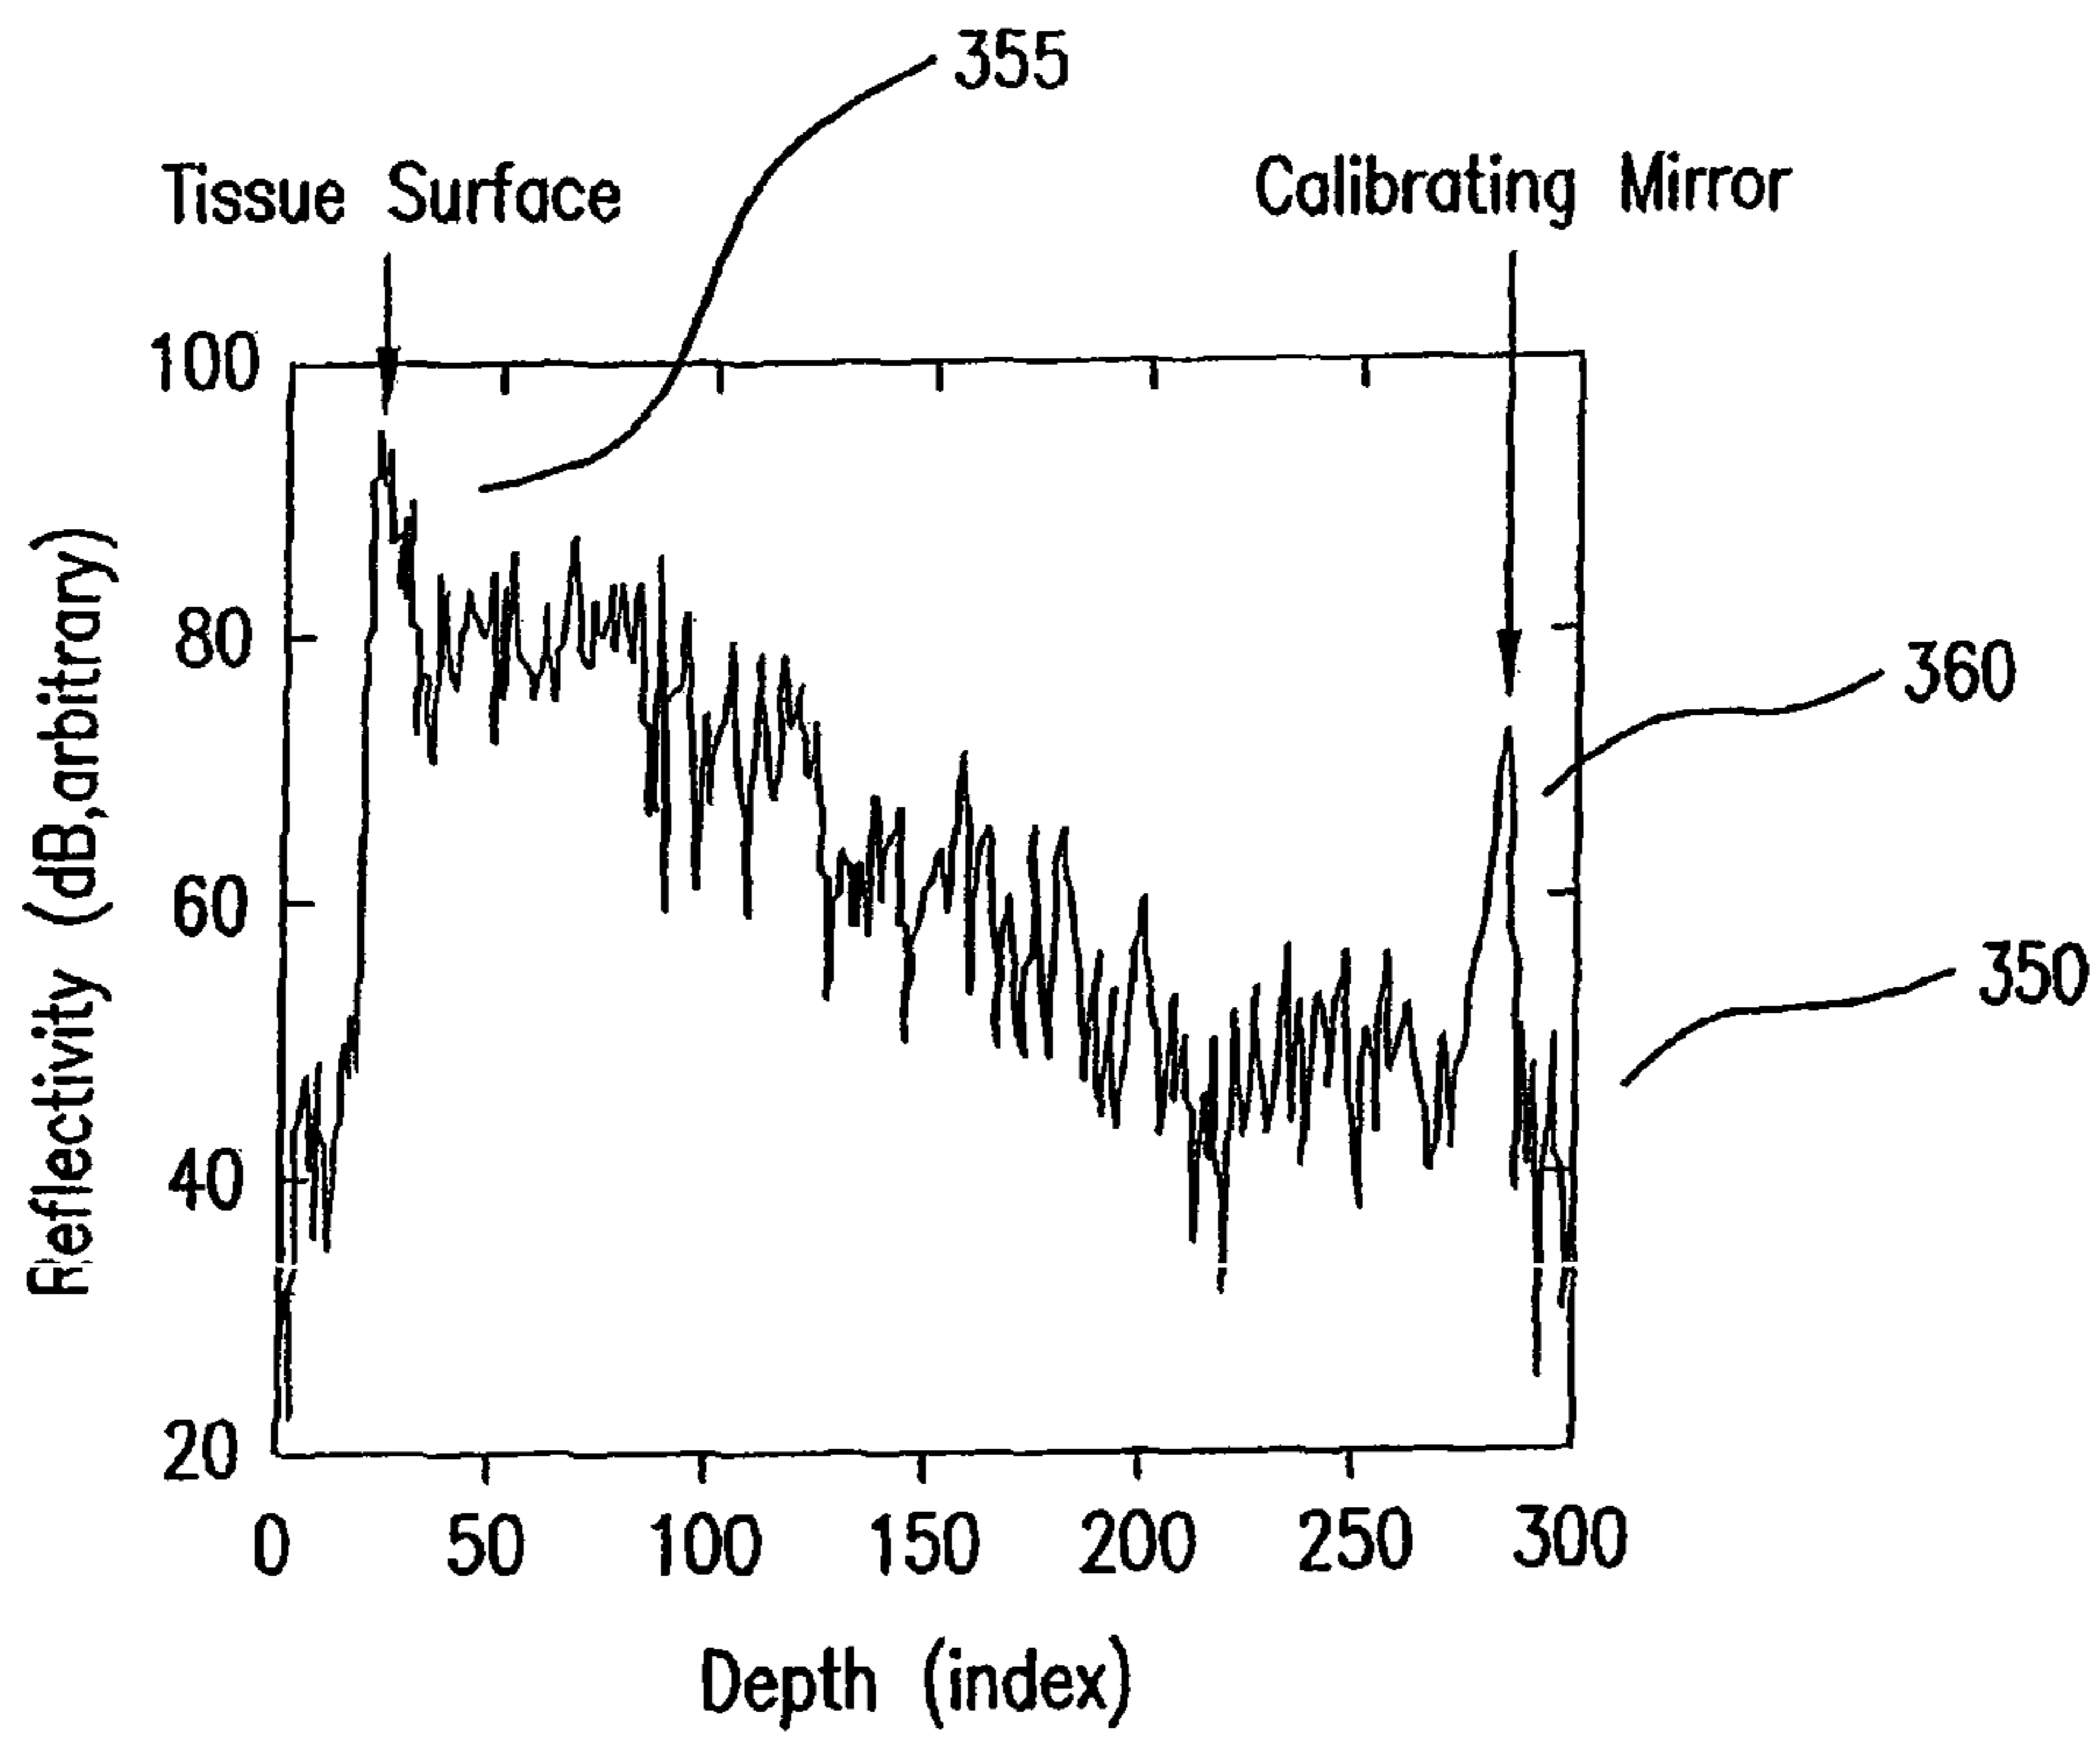


FIG. 3A

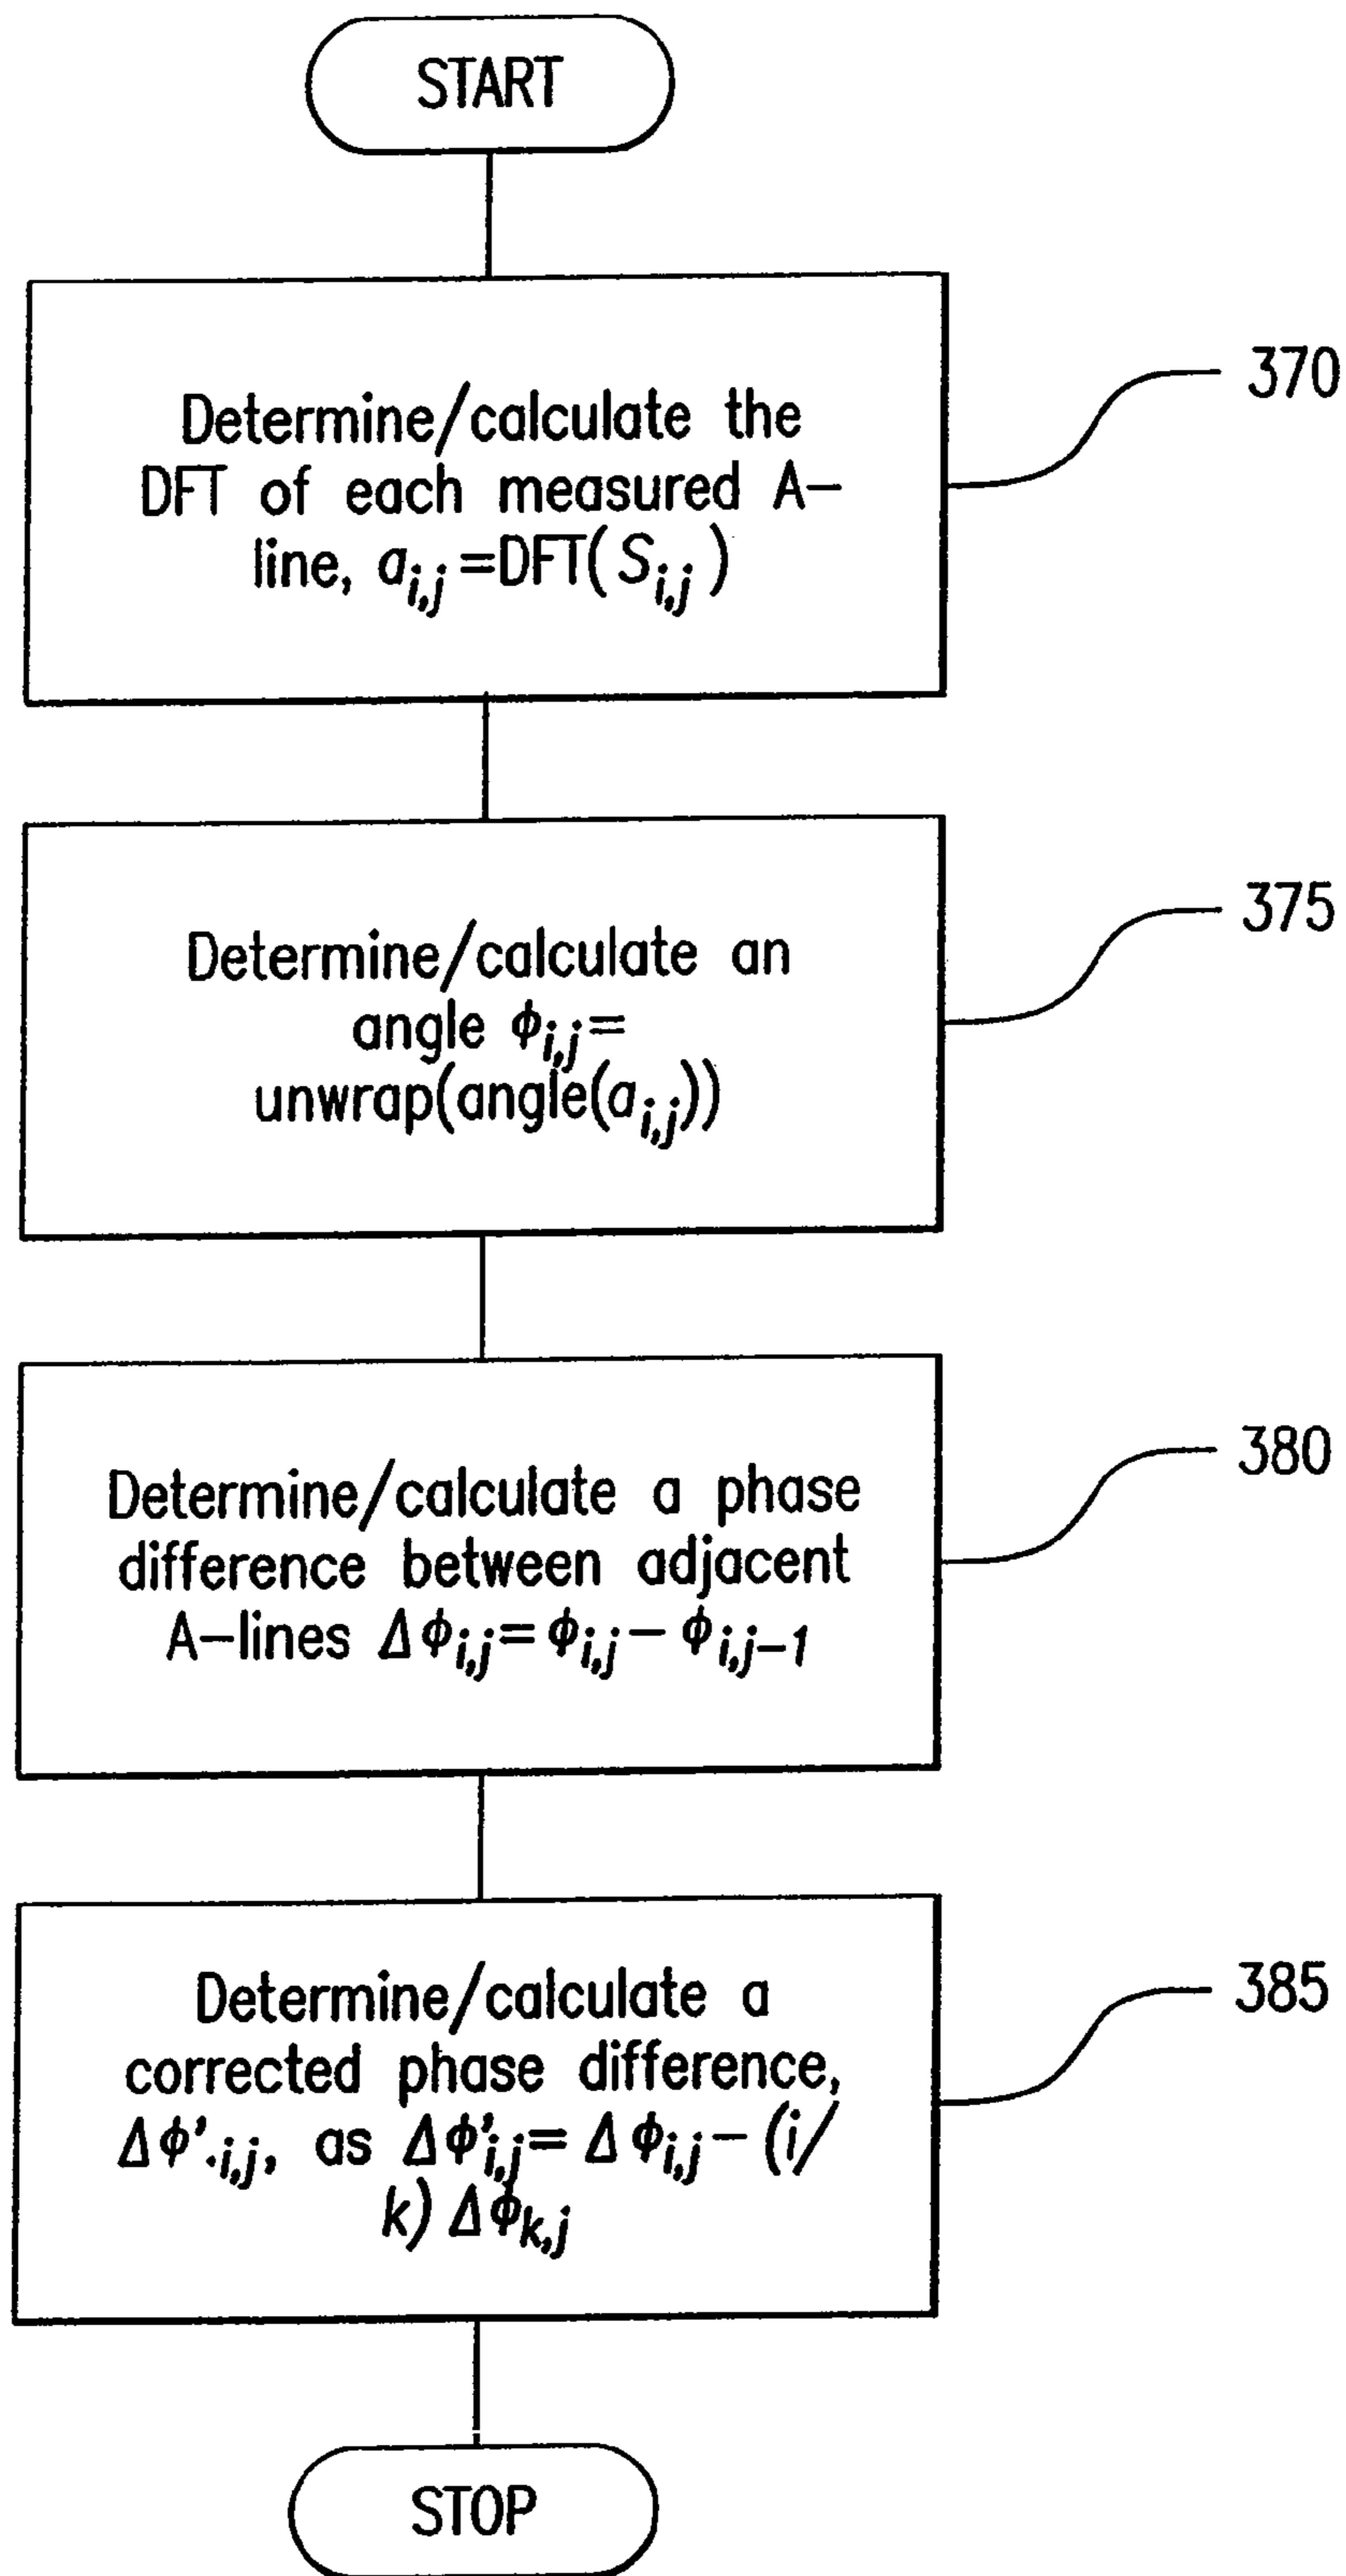


FIG. 3B

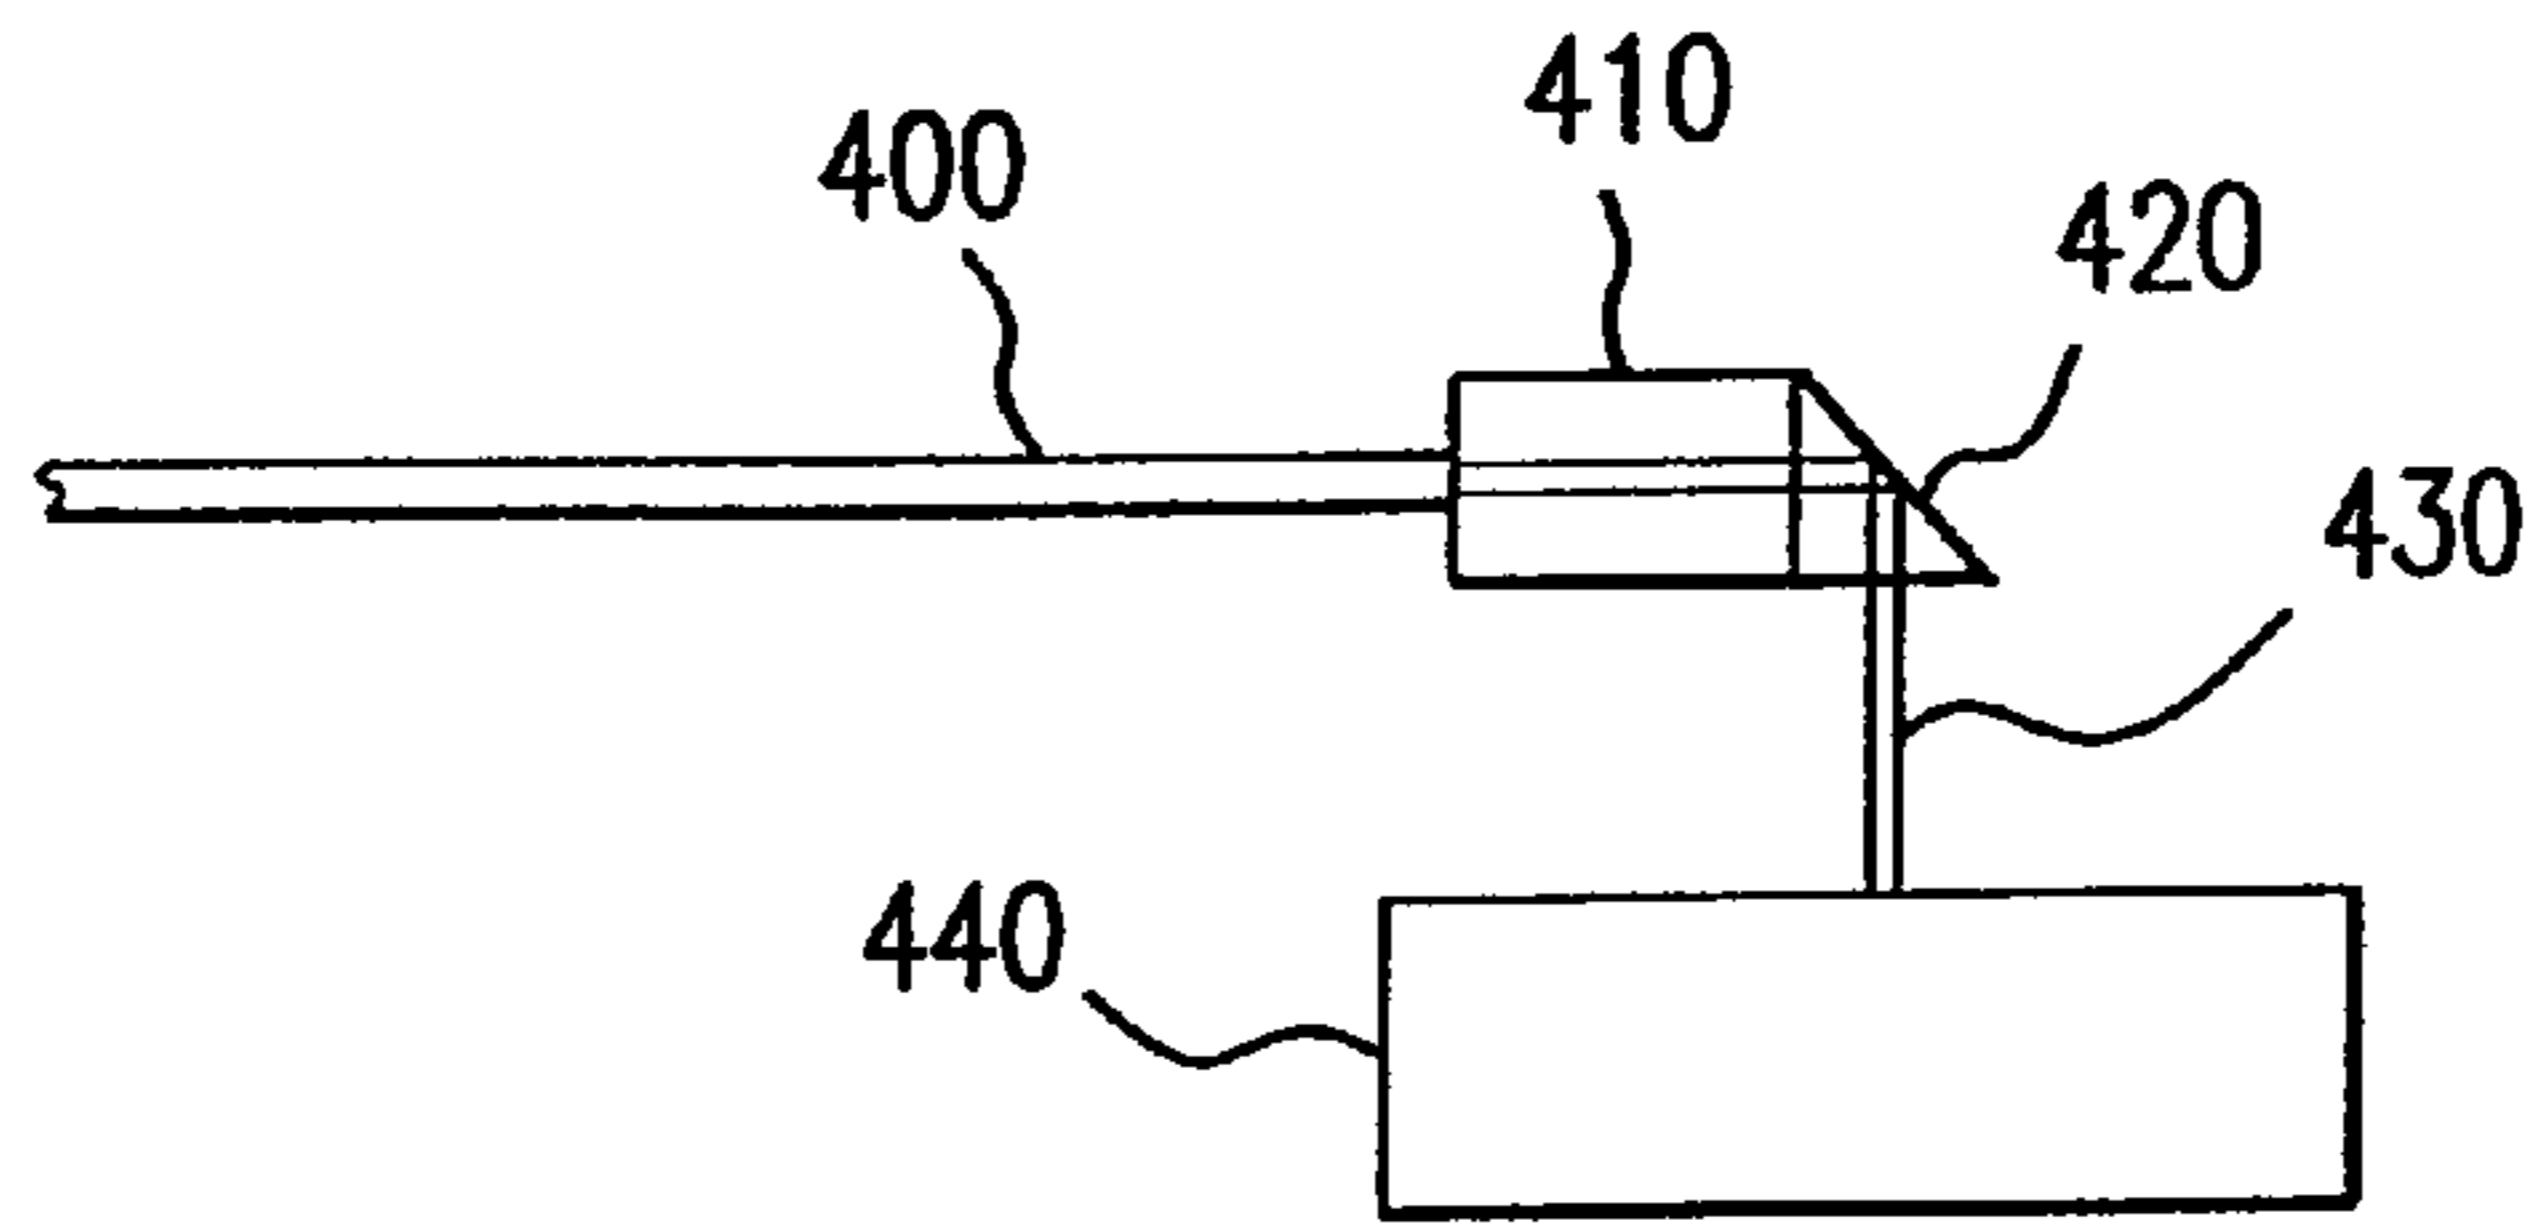


FIG. 4
PRIOR ART

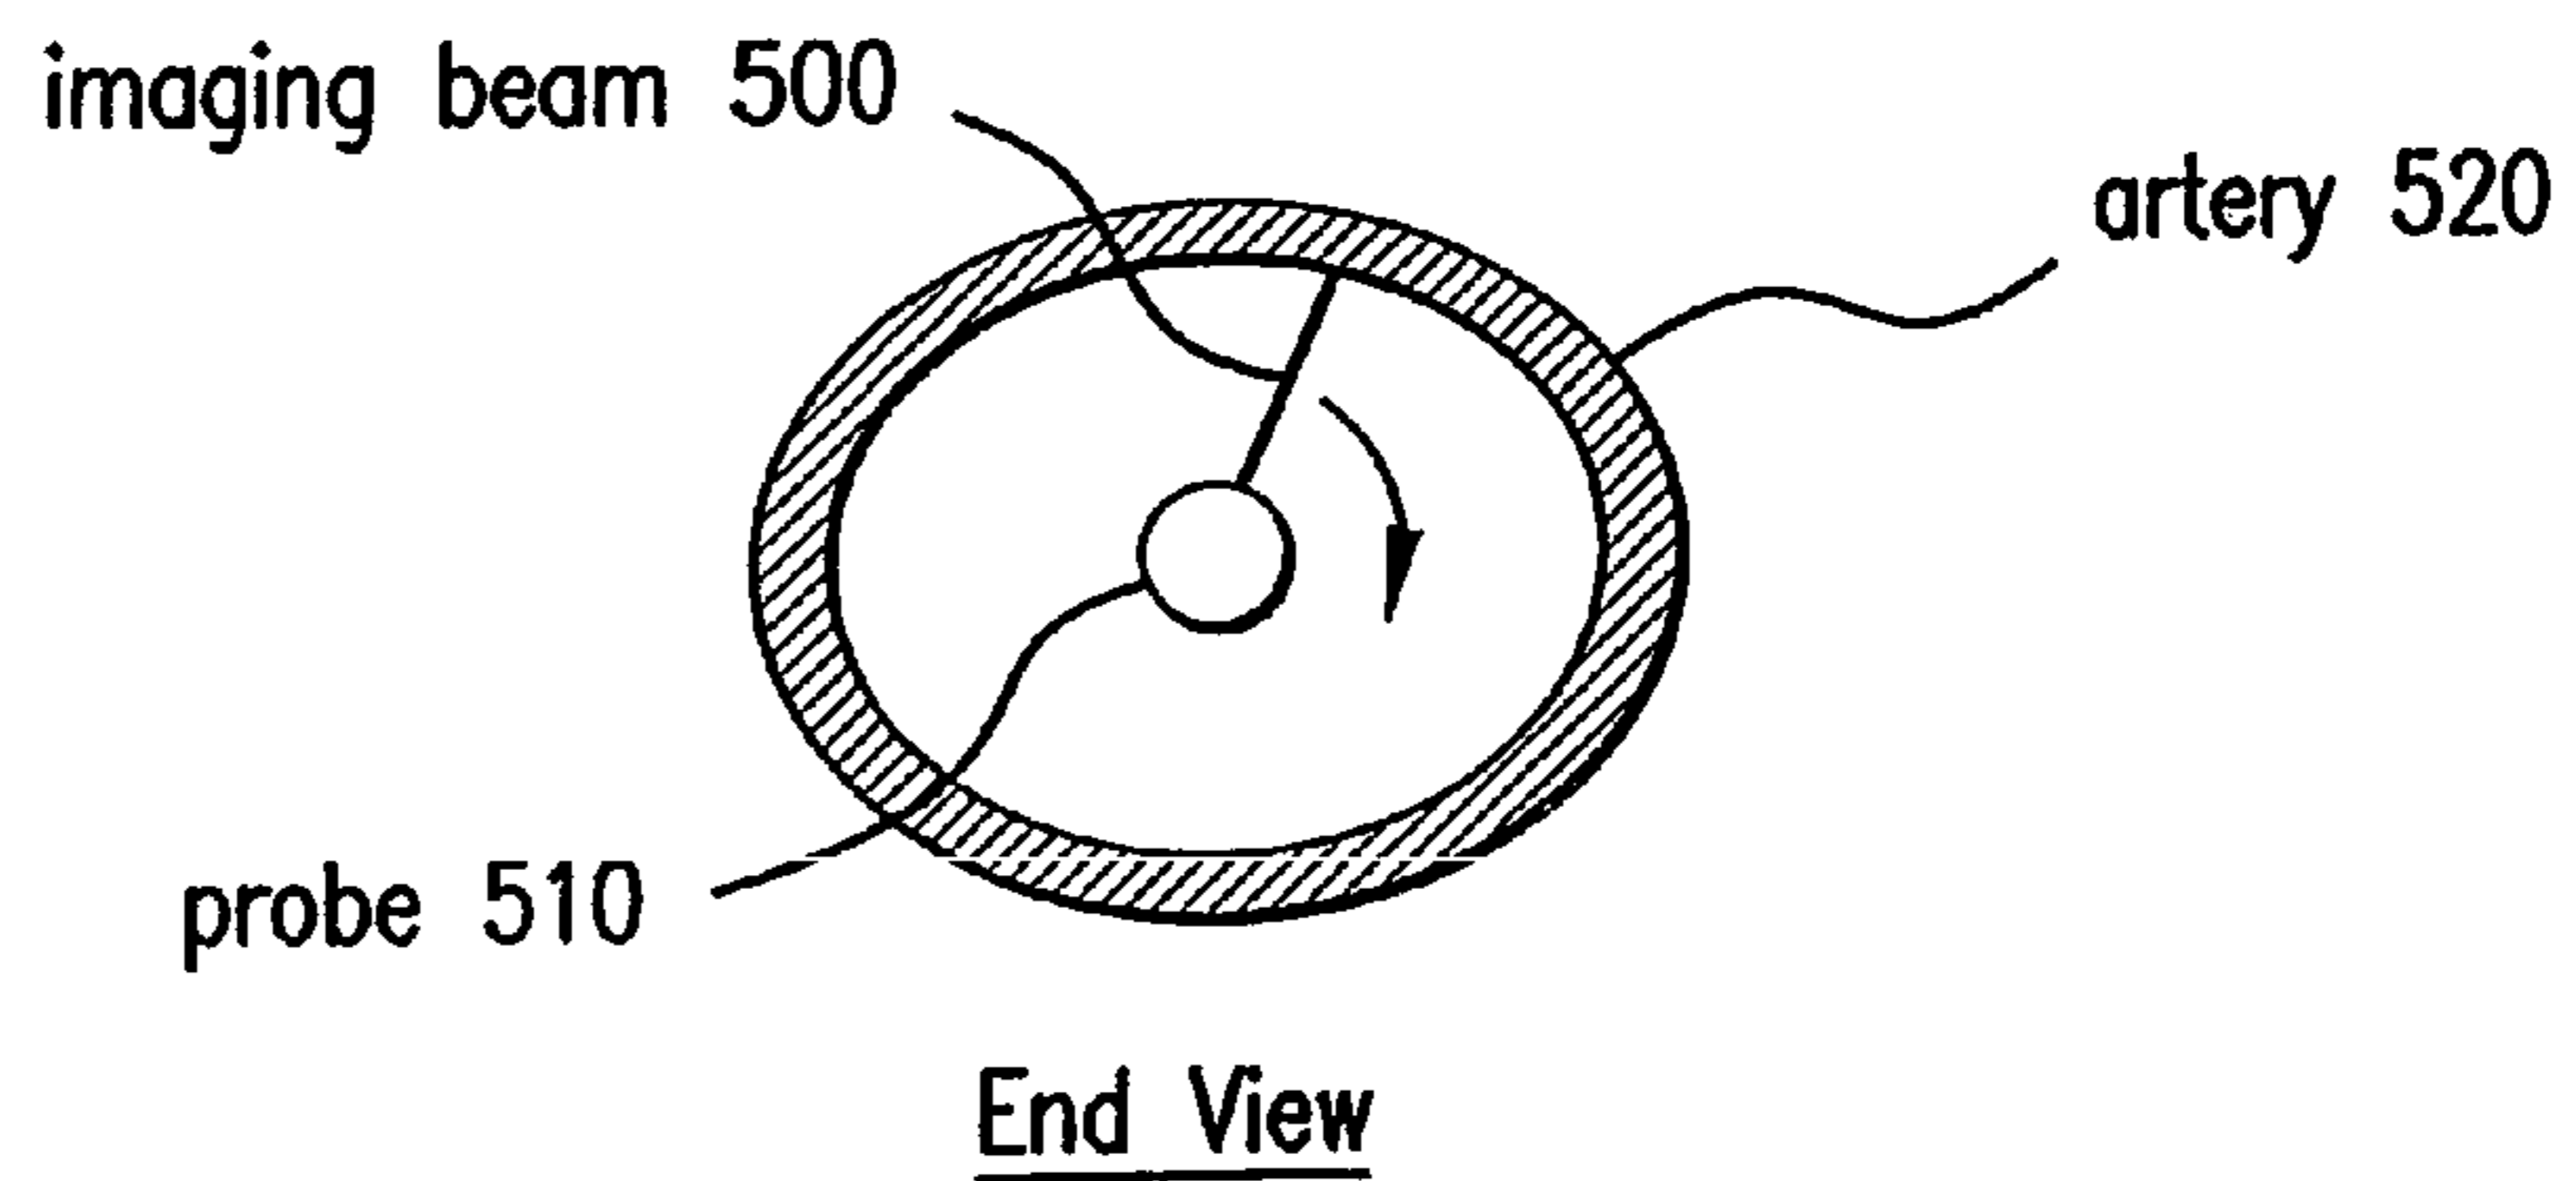
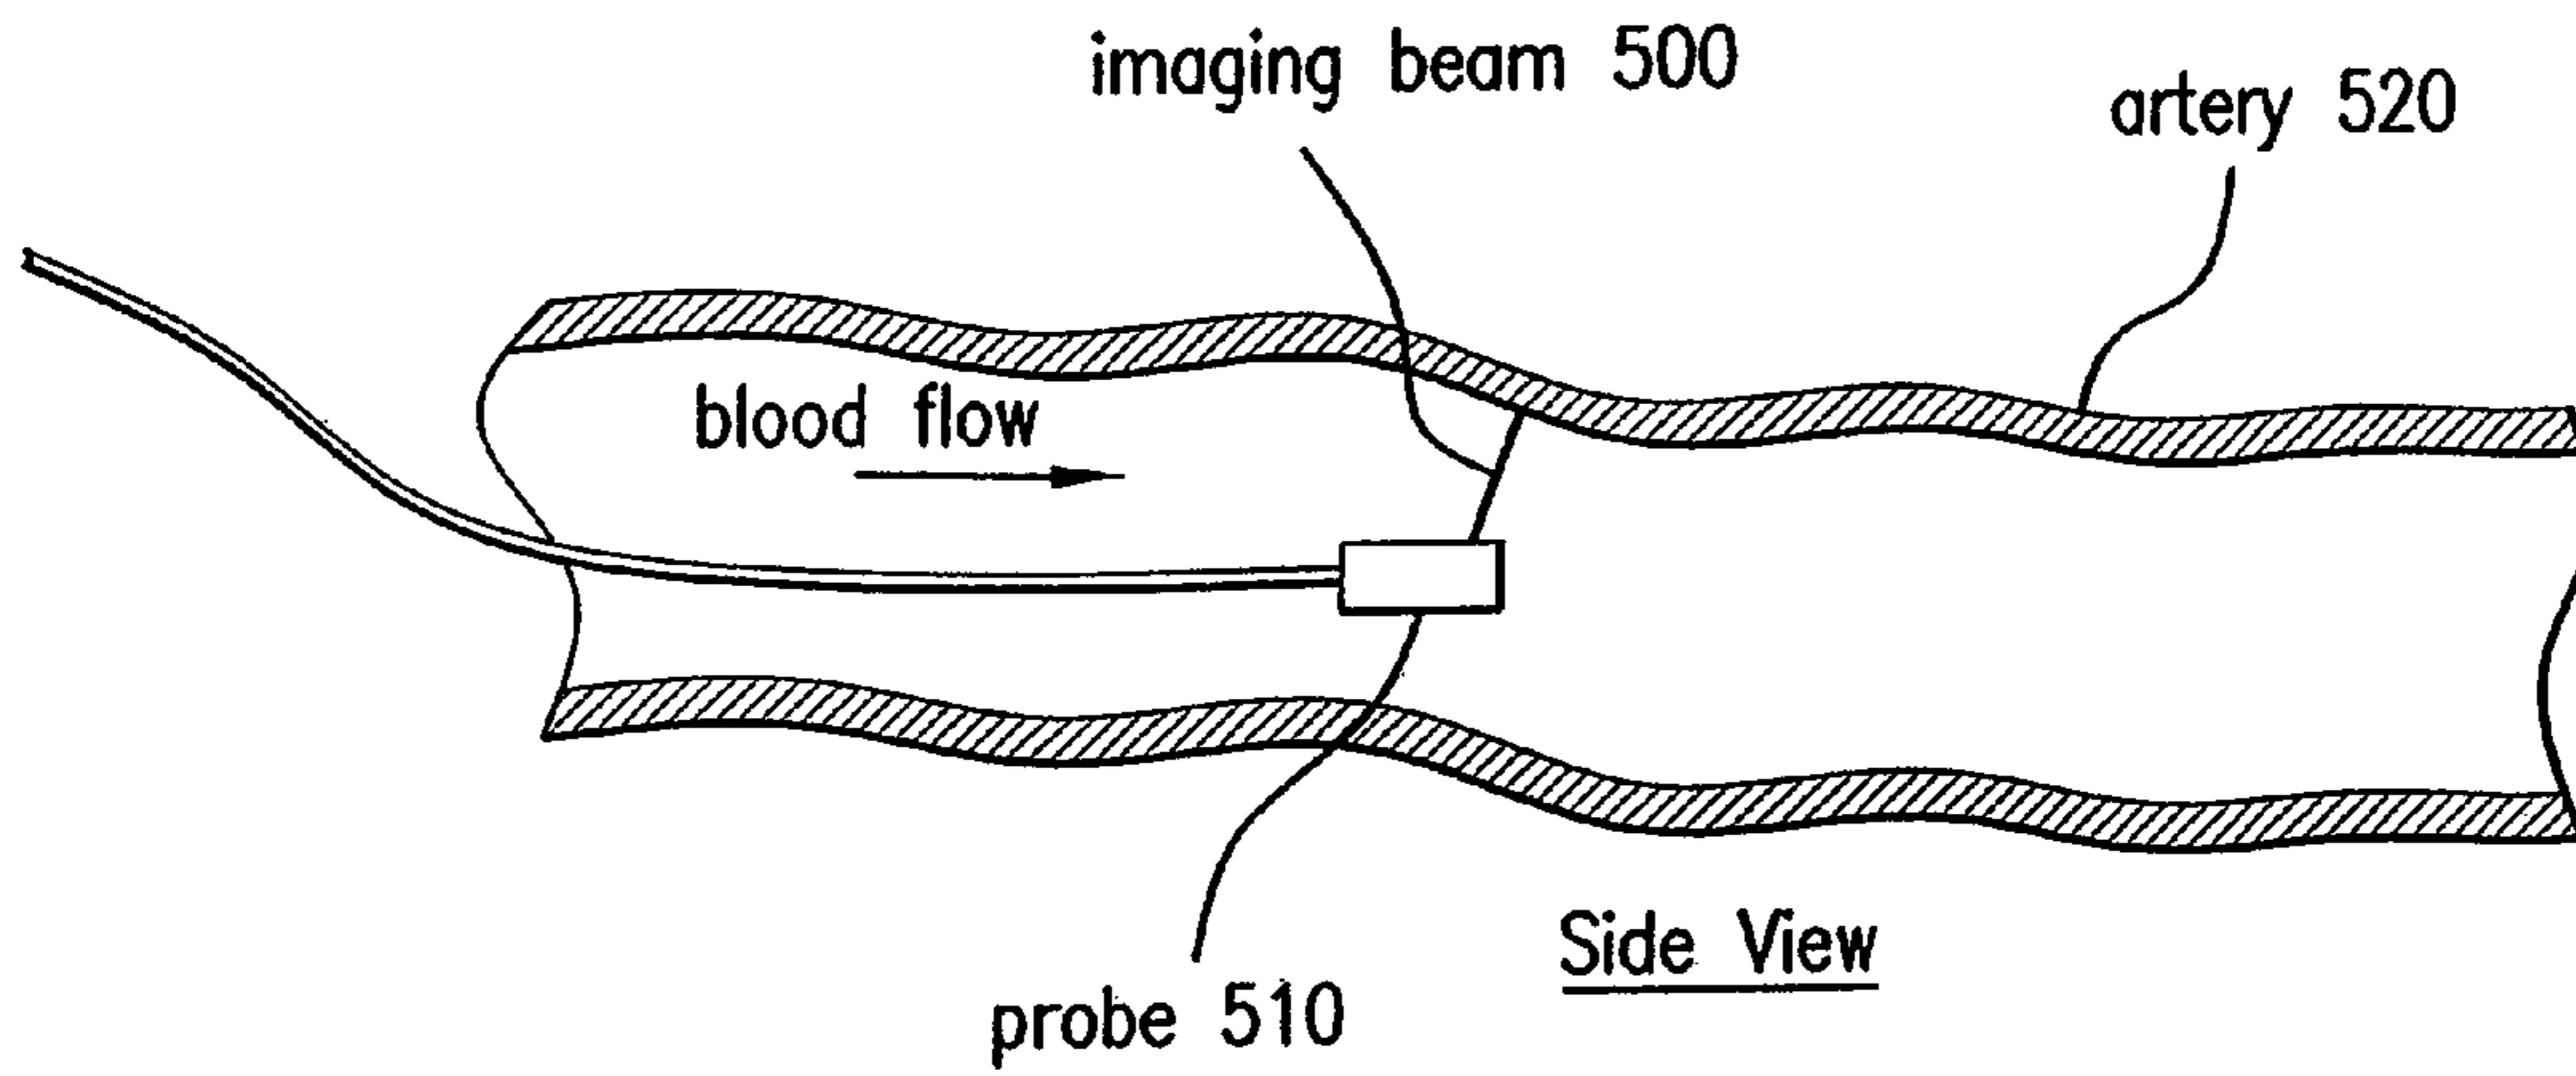


FIG. 5

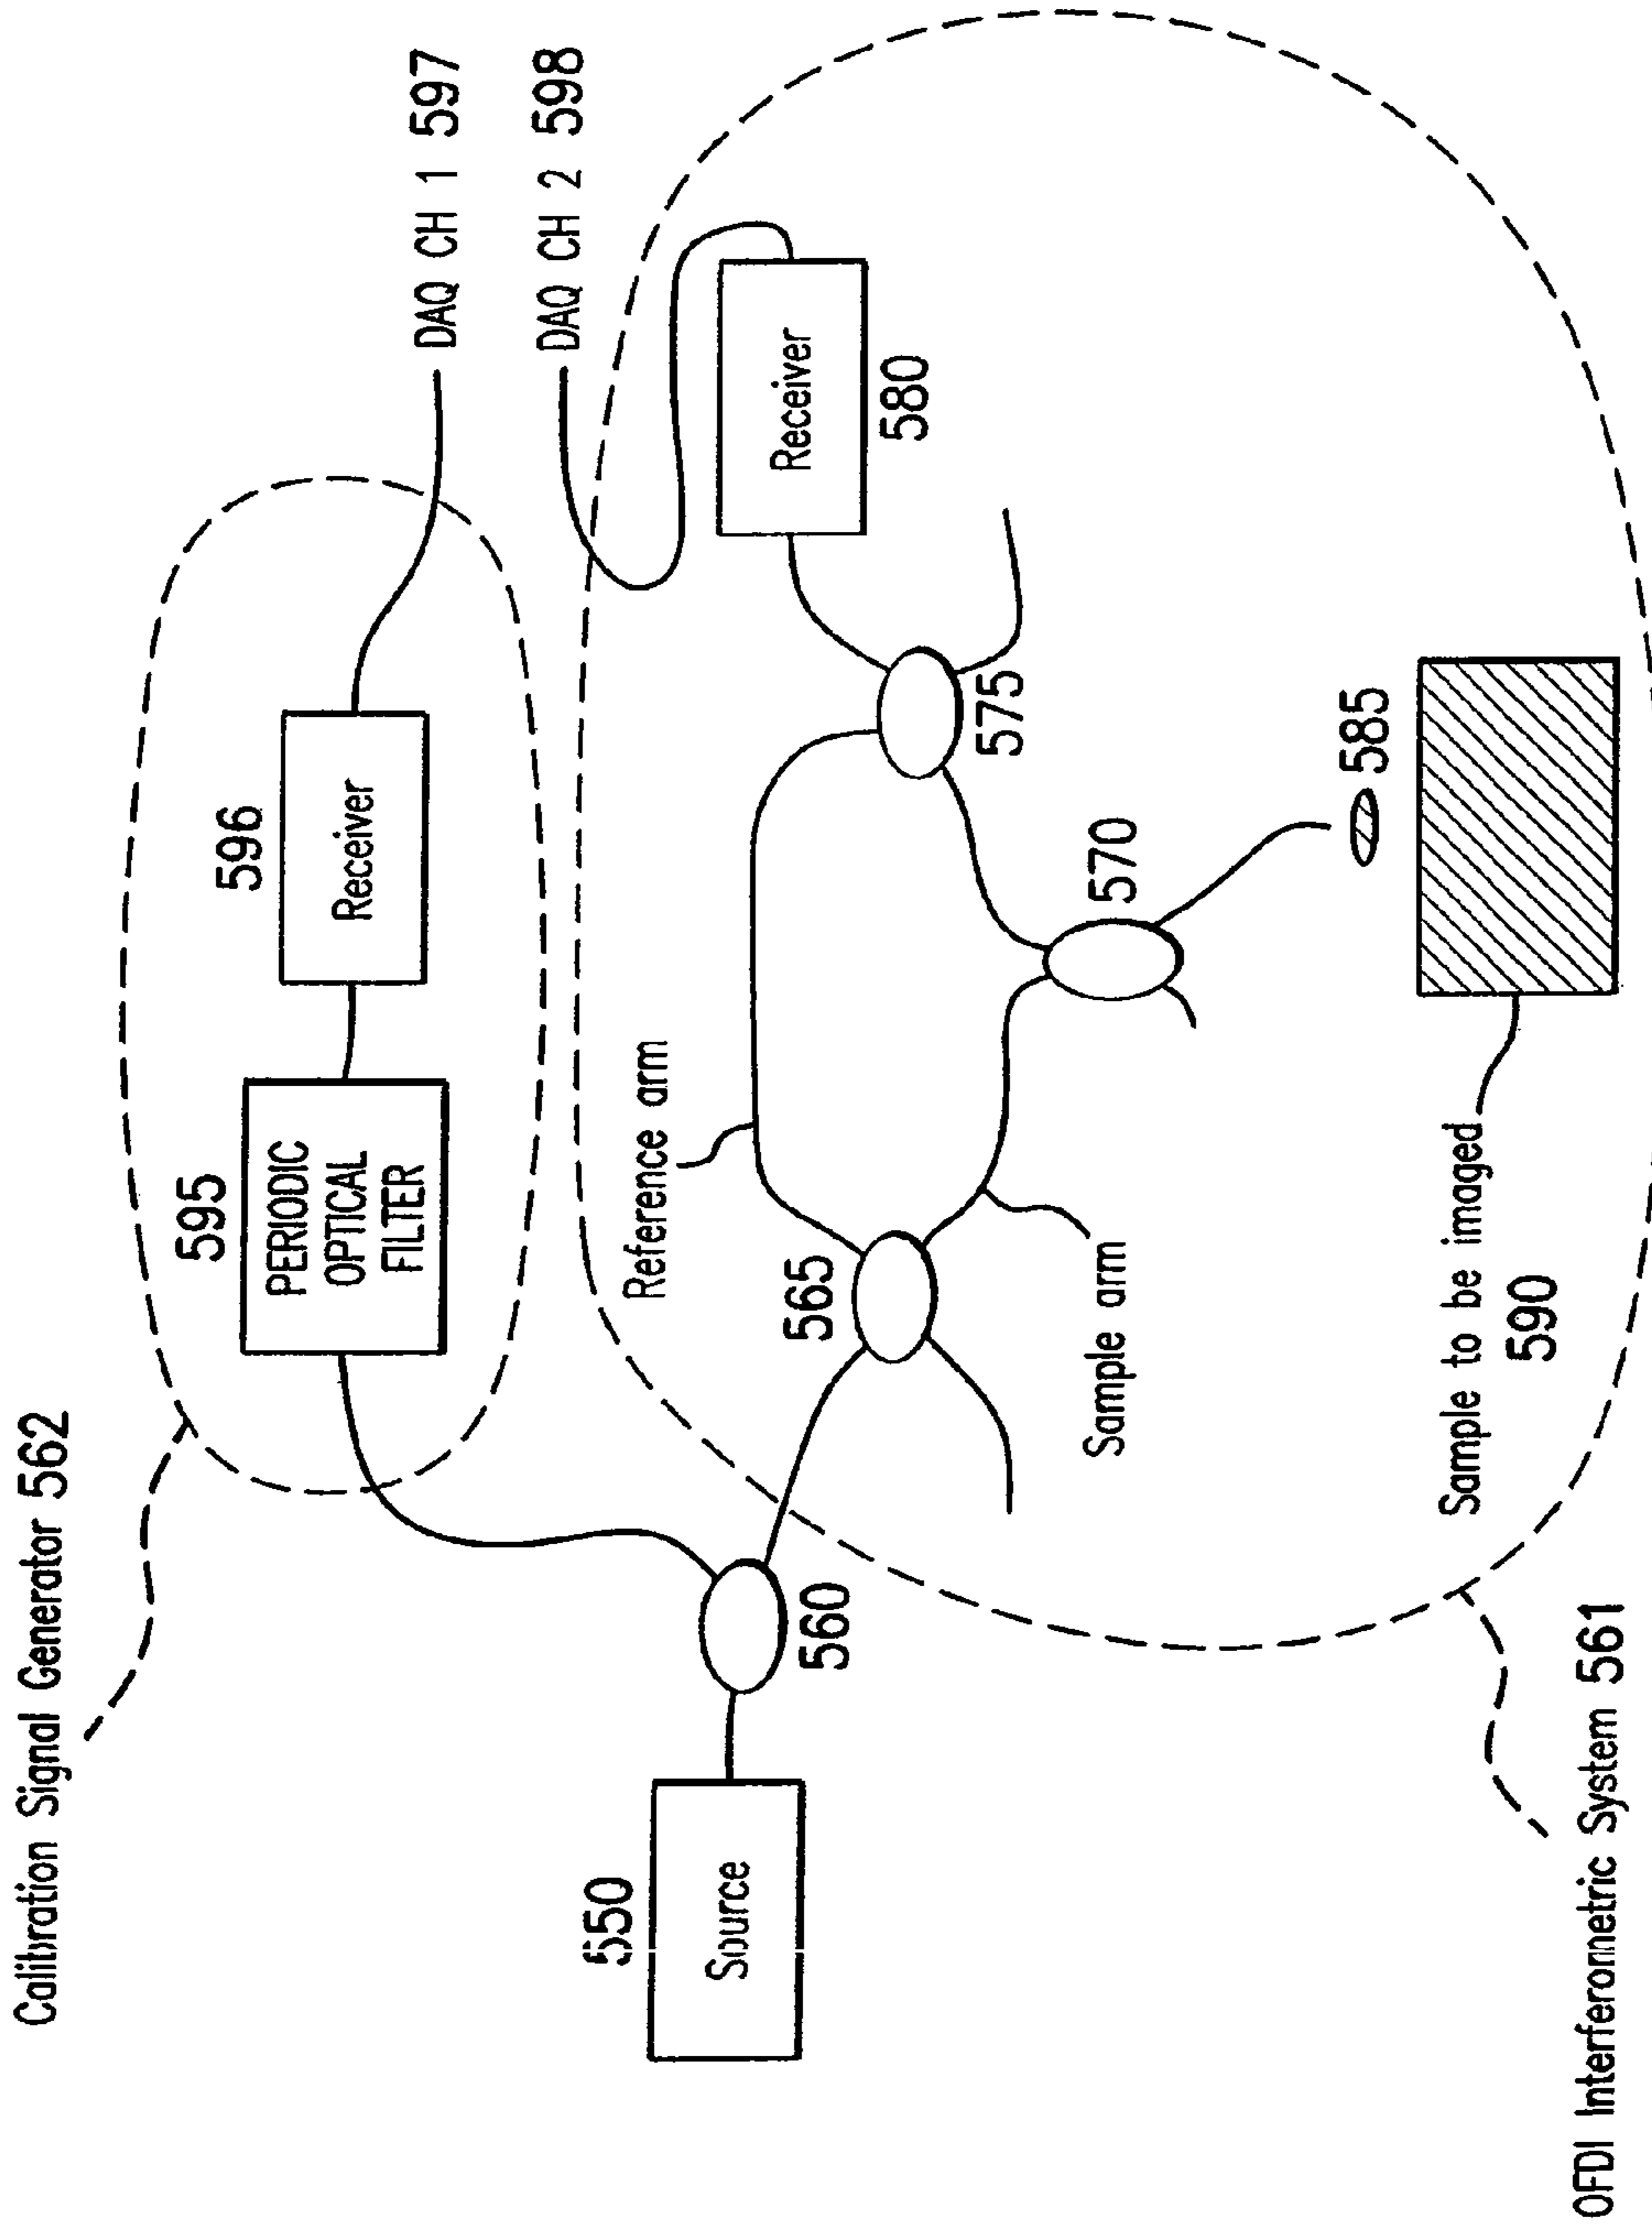


FIG.6

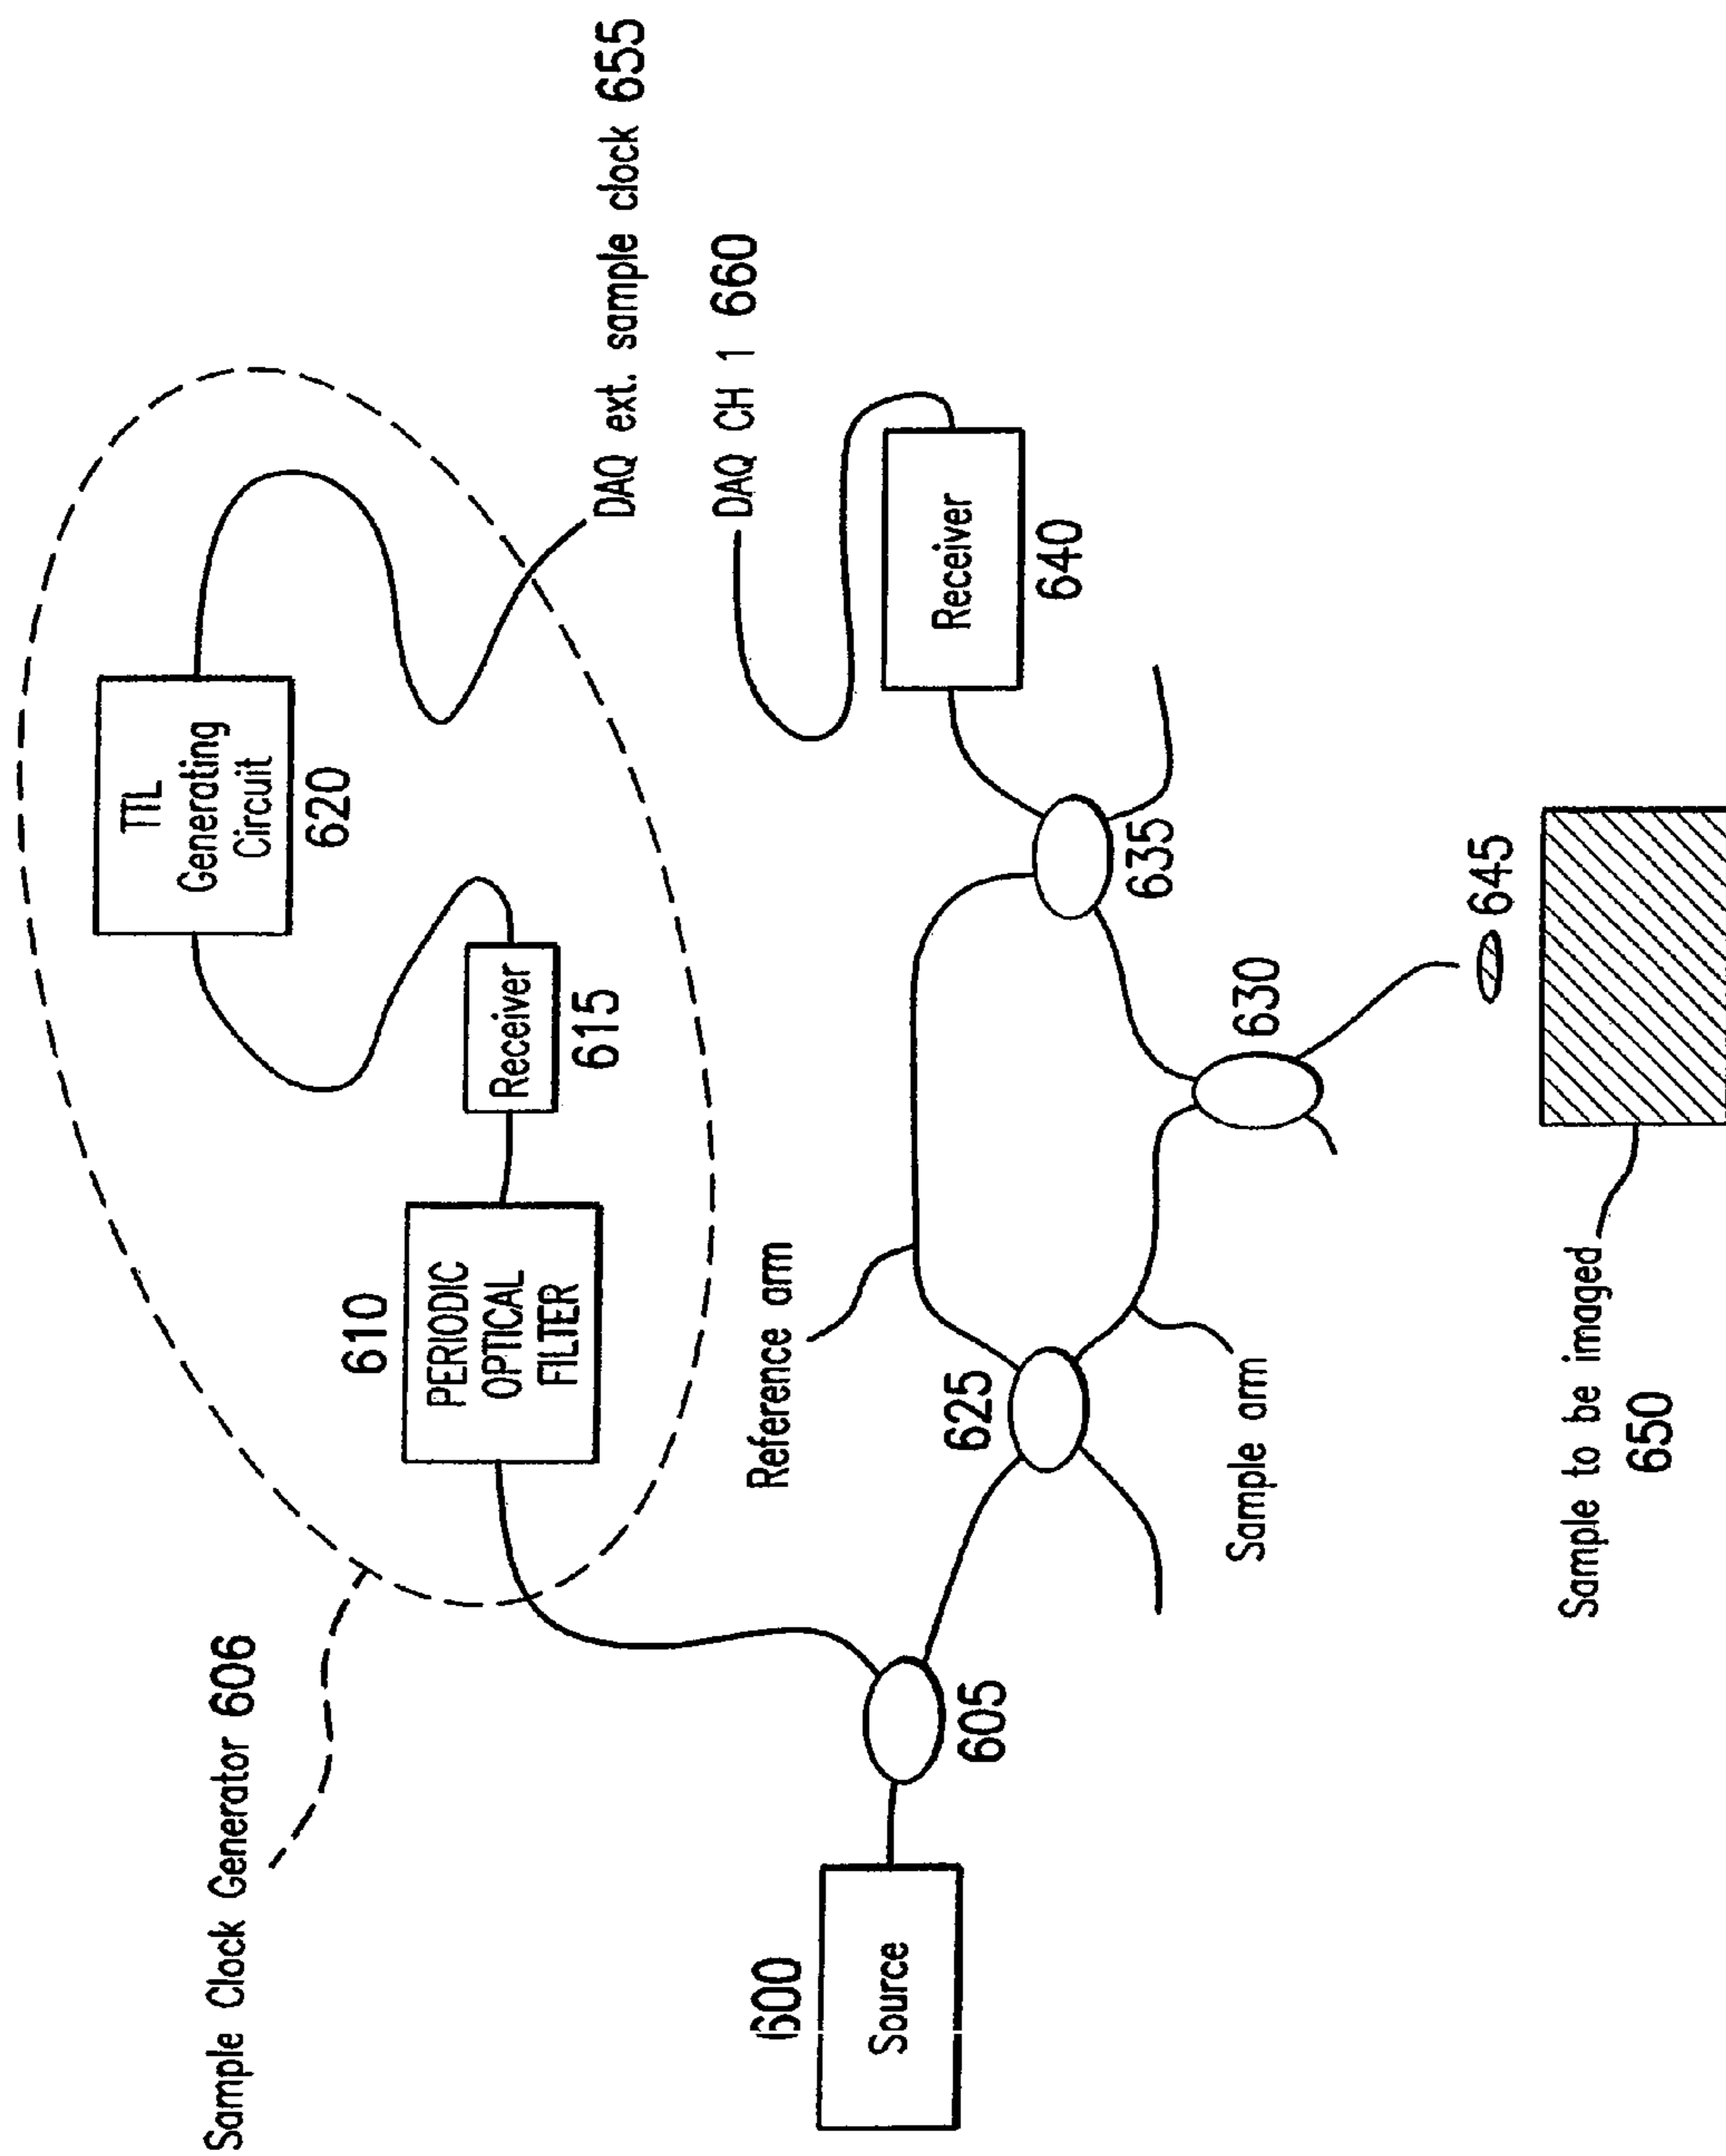


FIG. 7

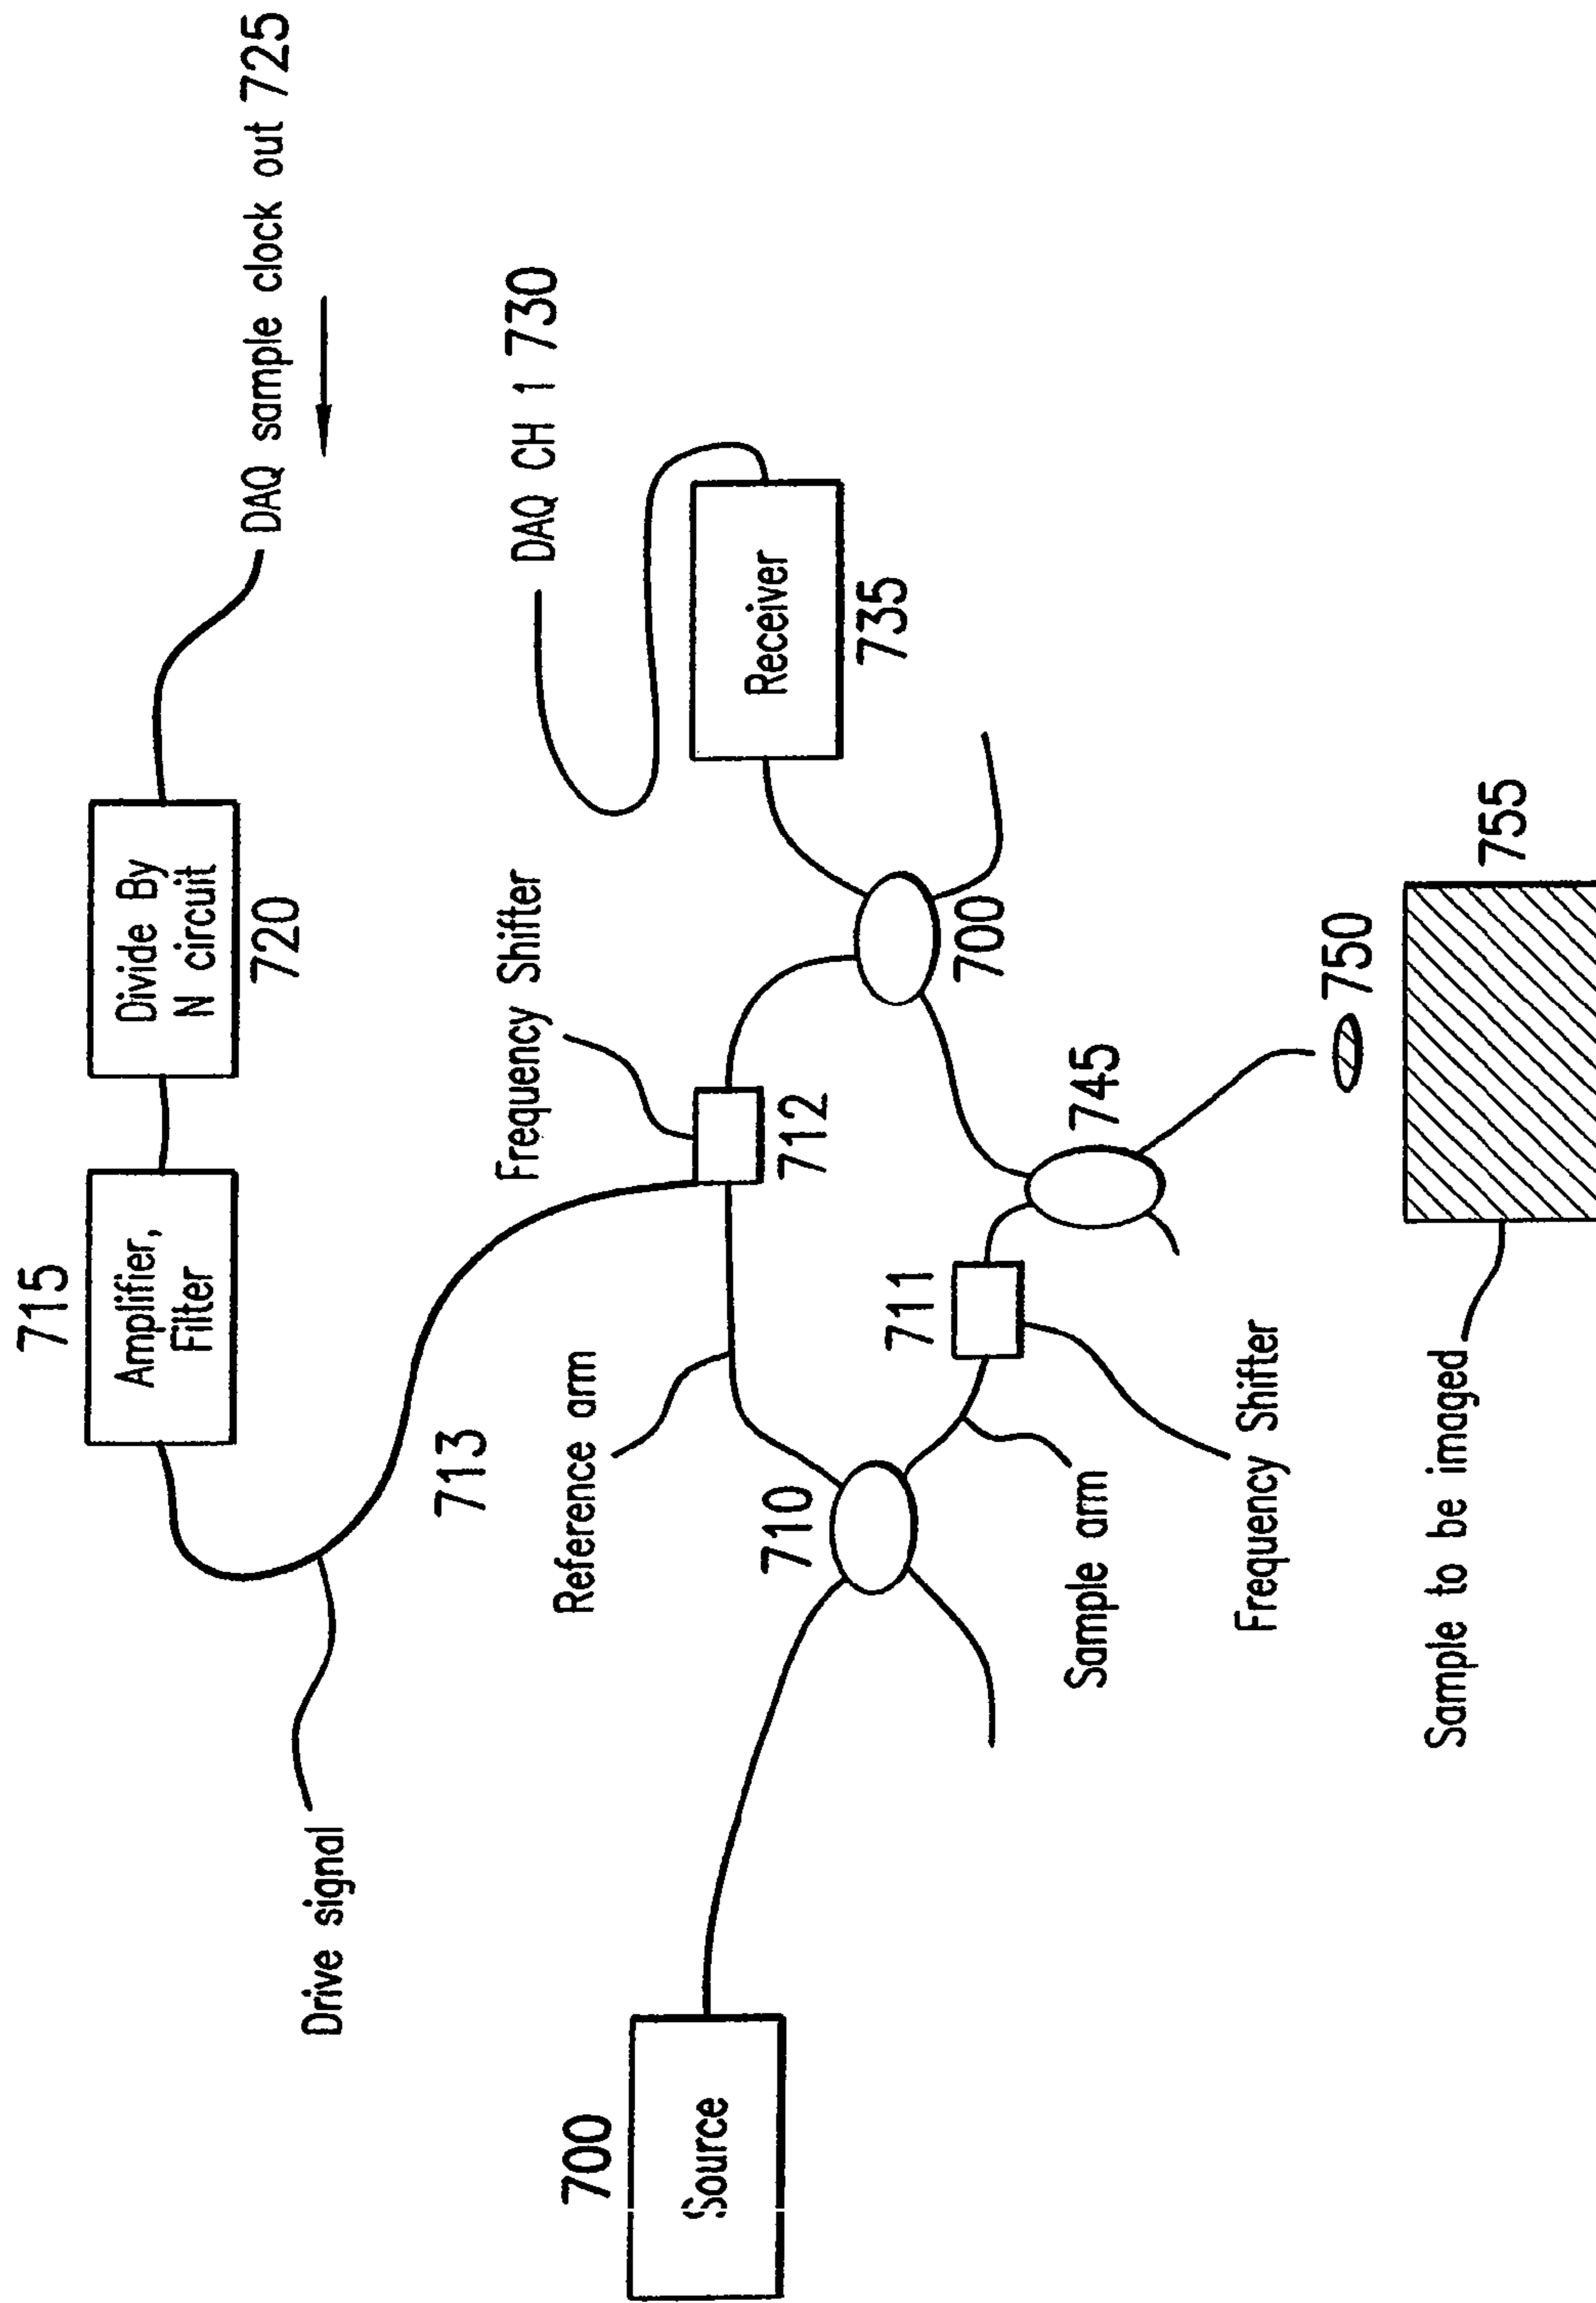


FIG. 8


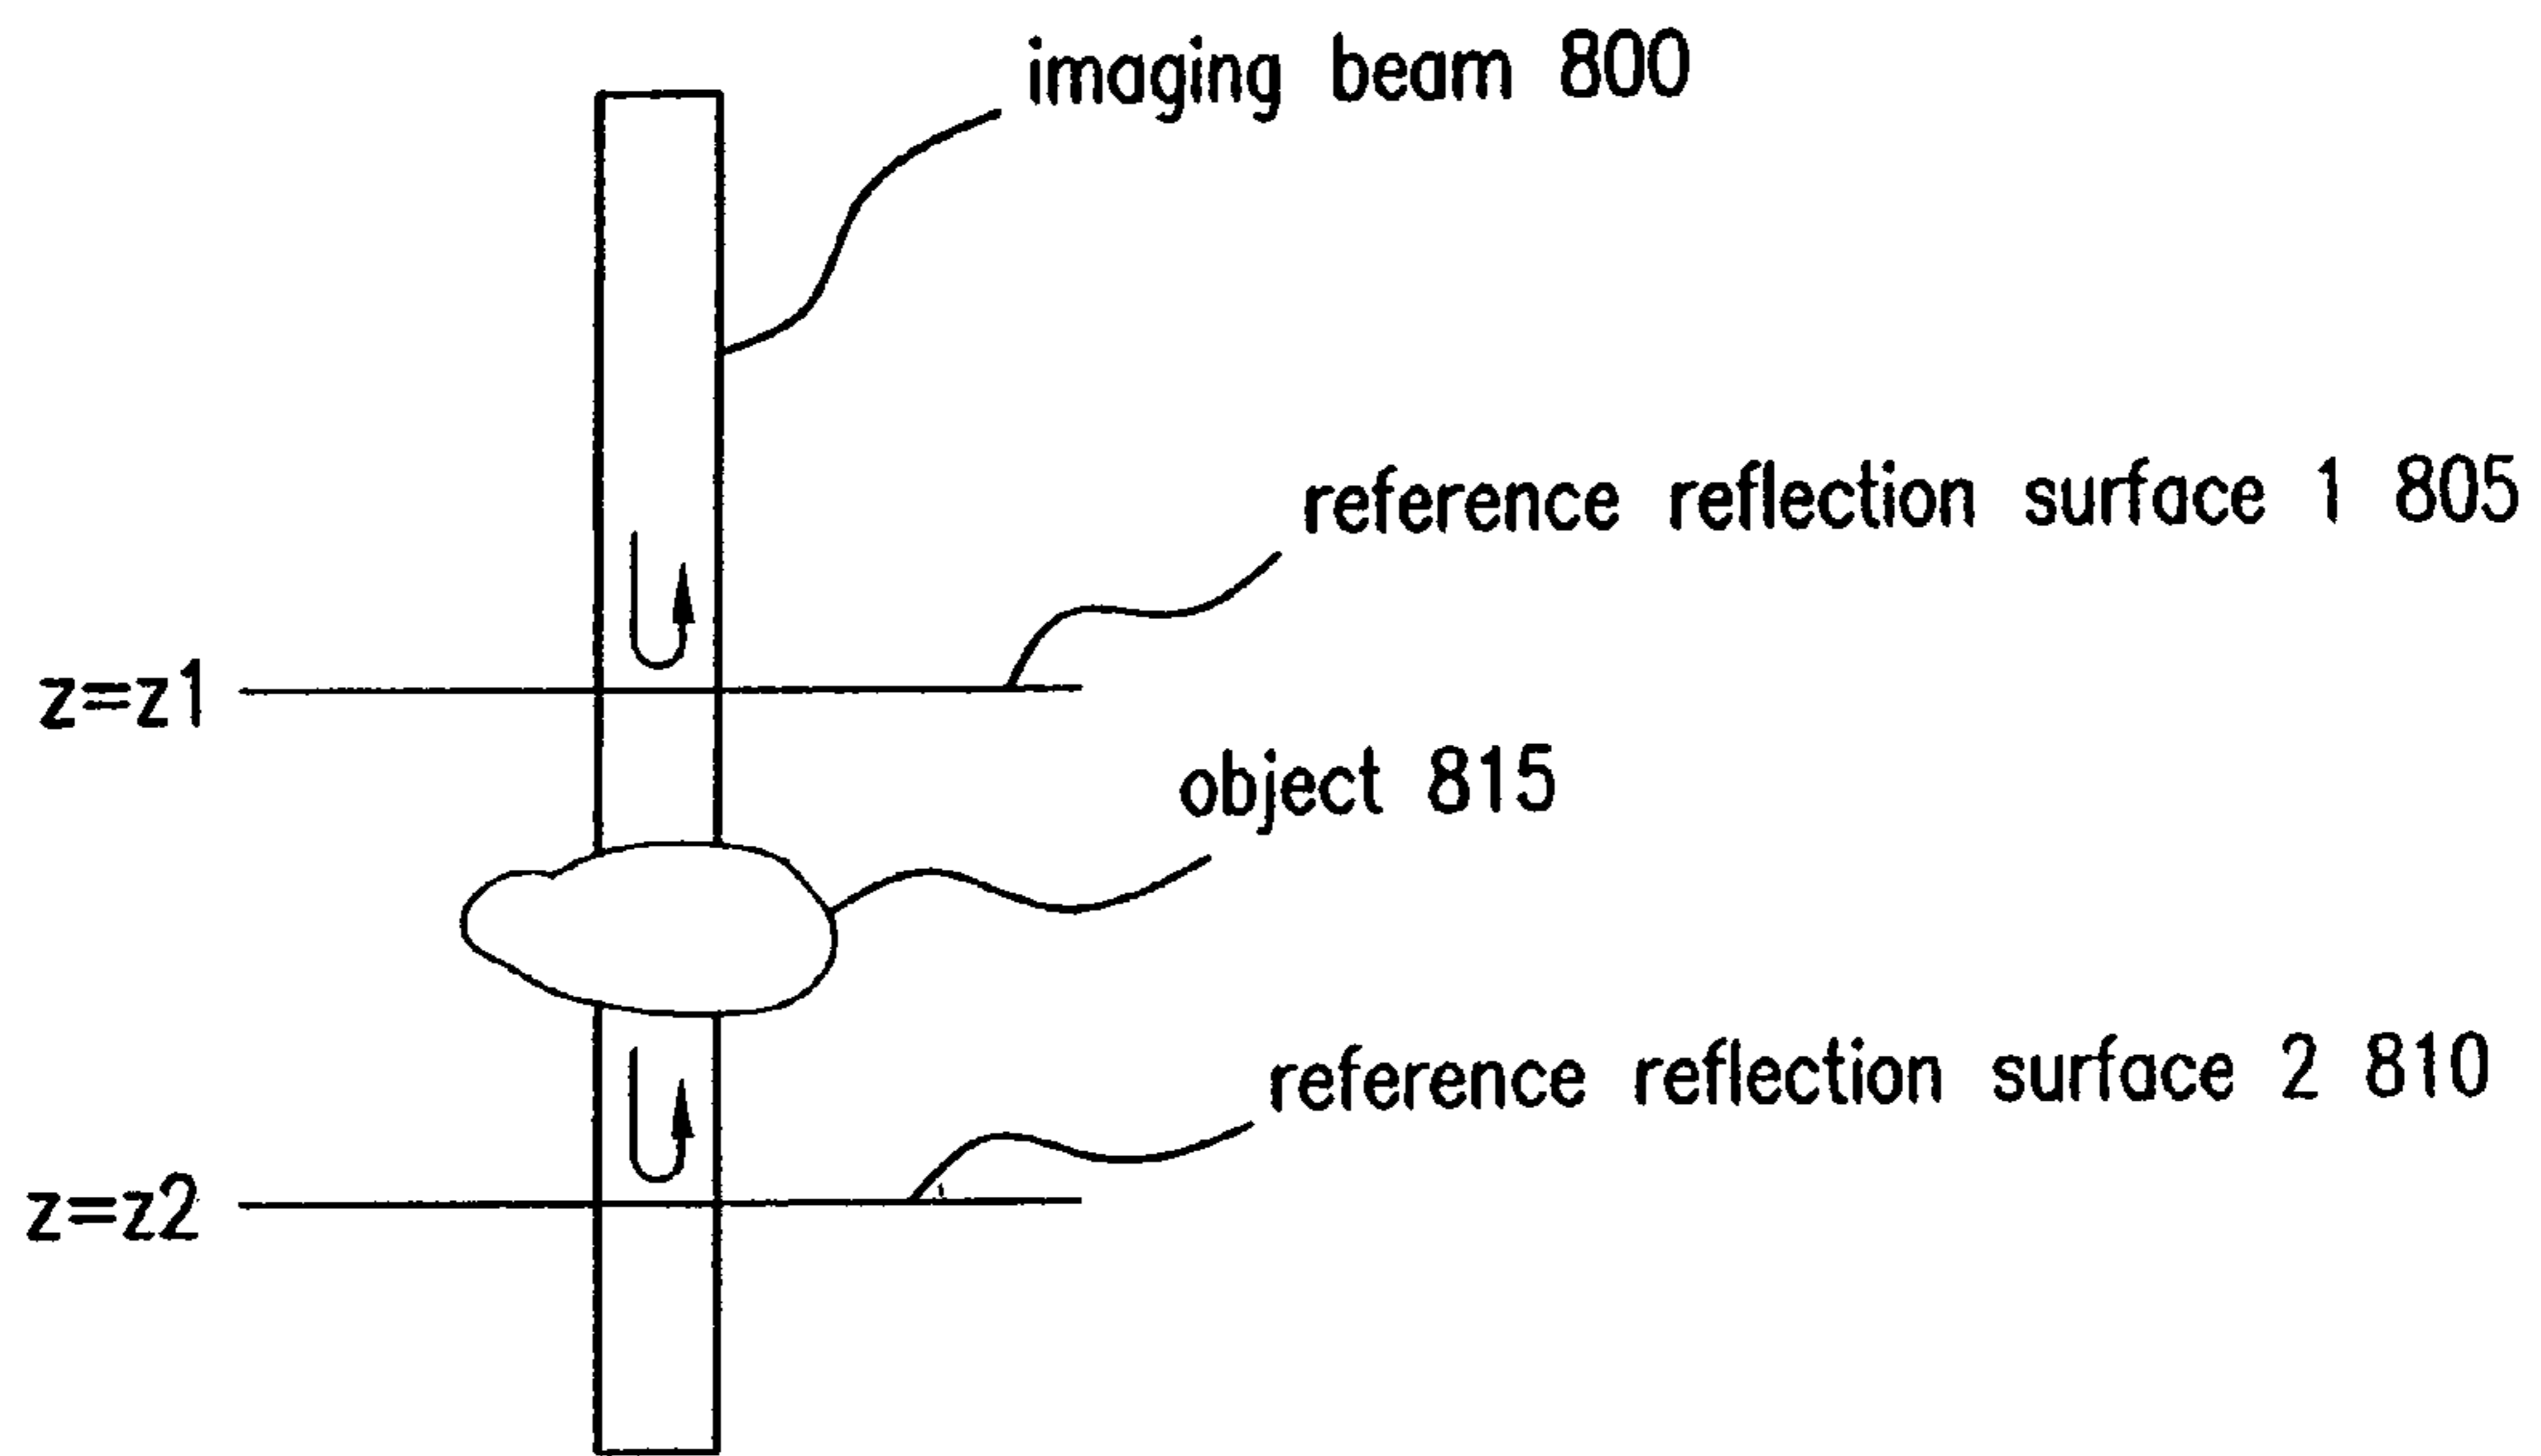


FIG. 9

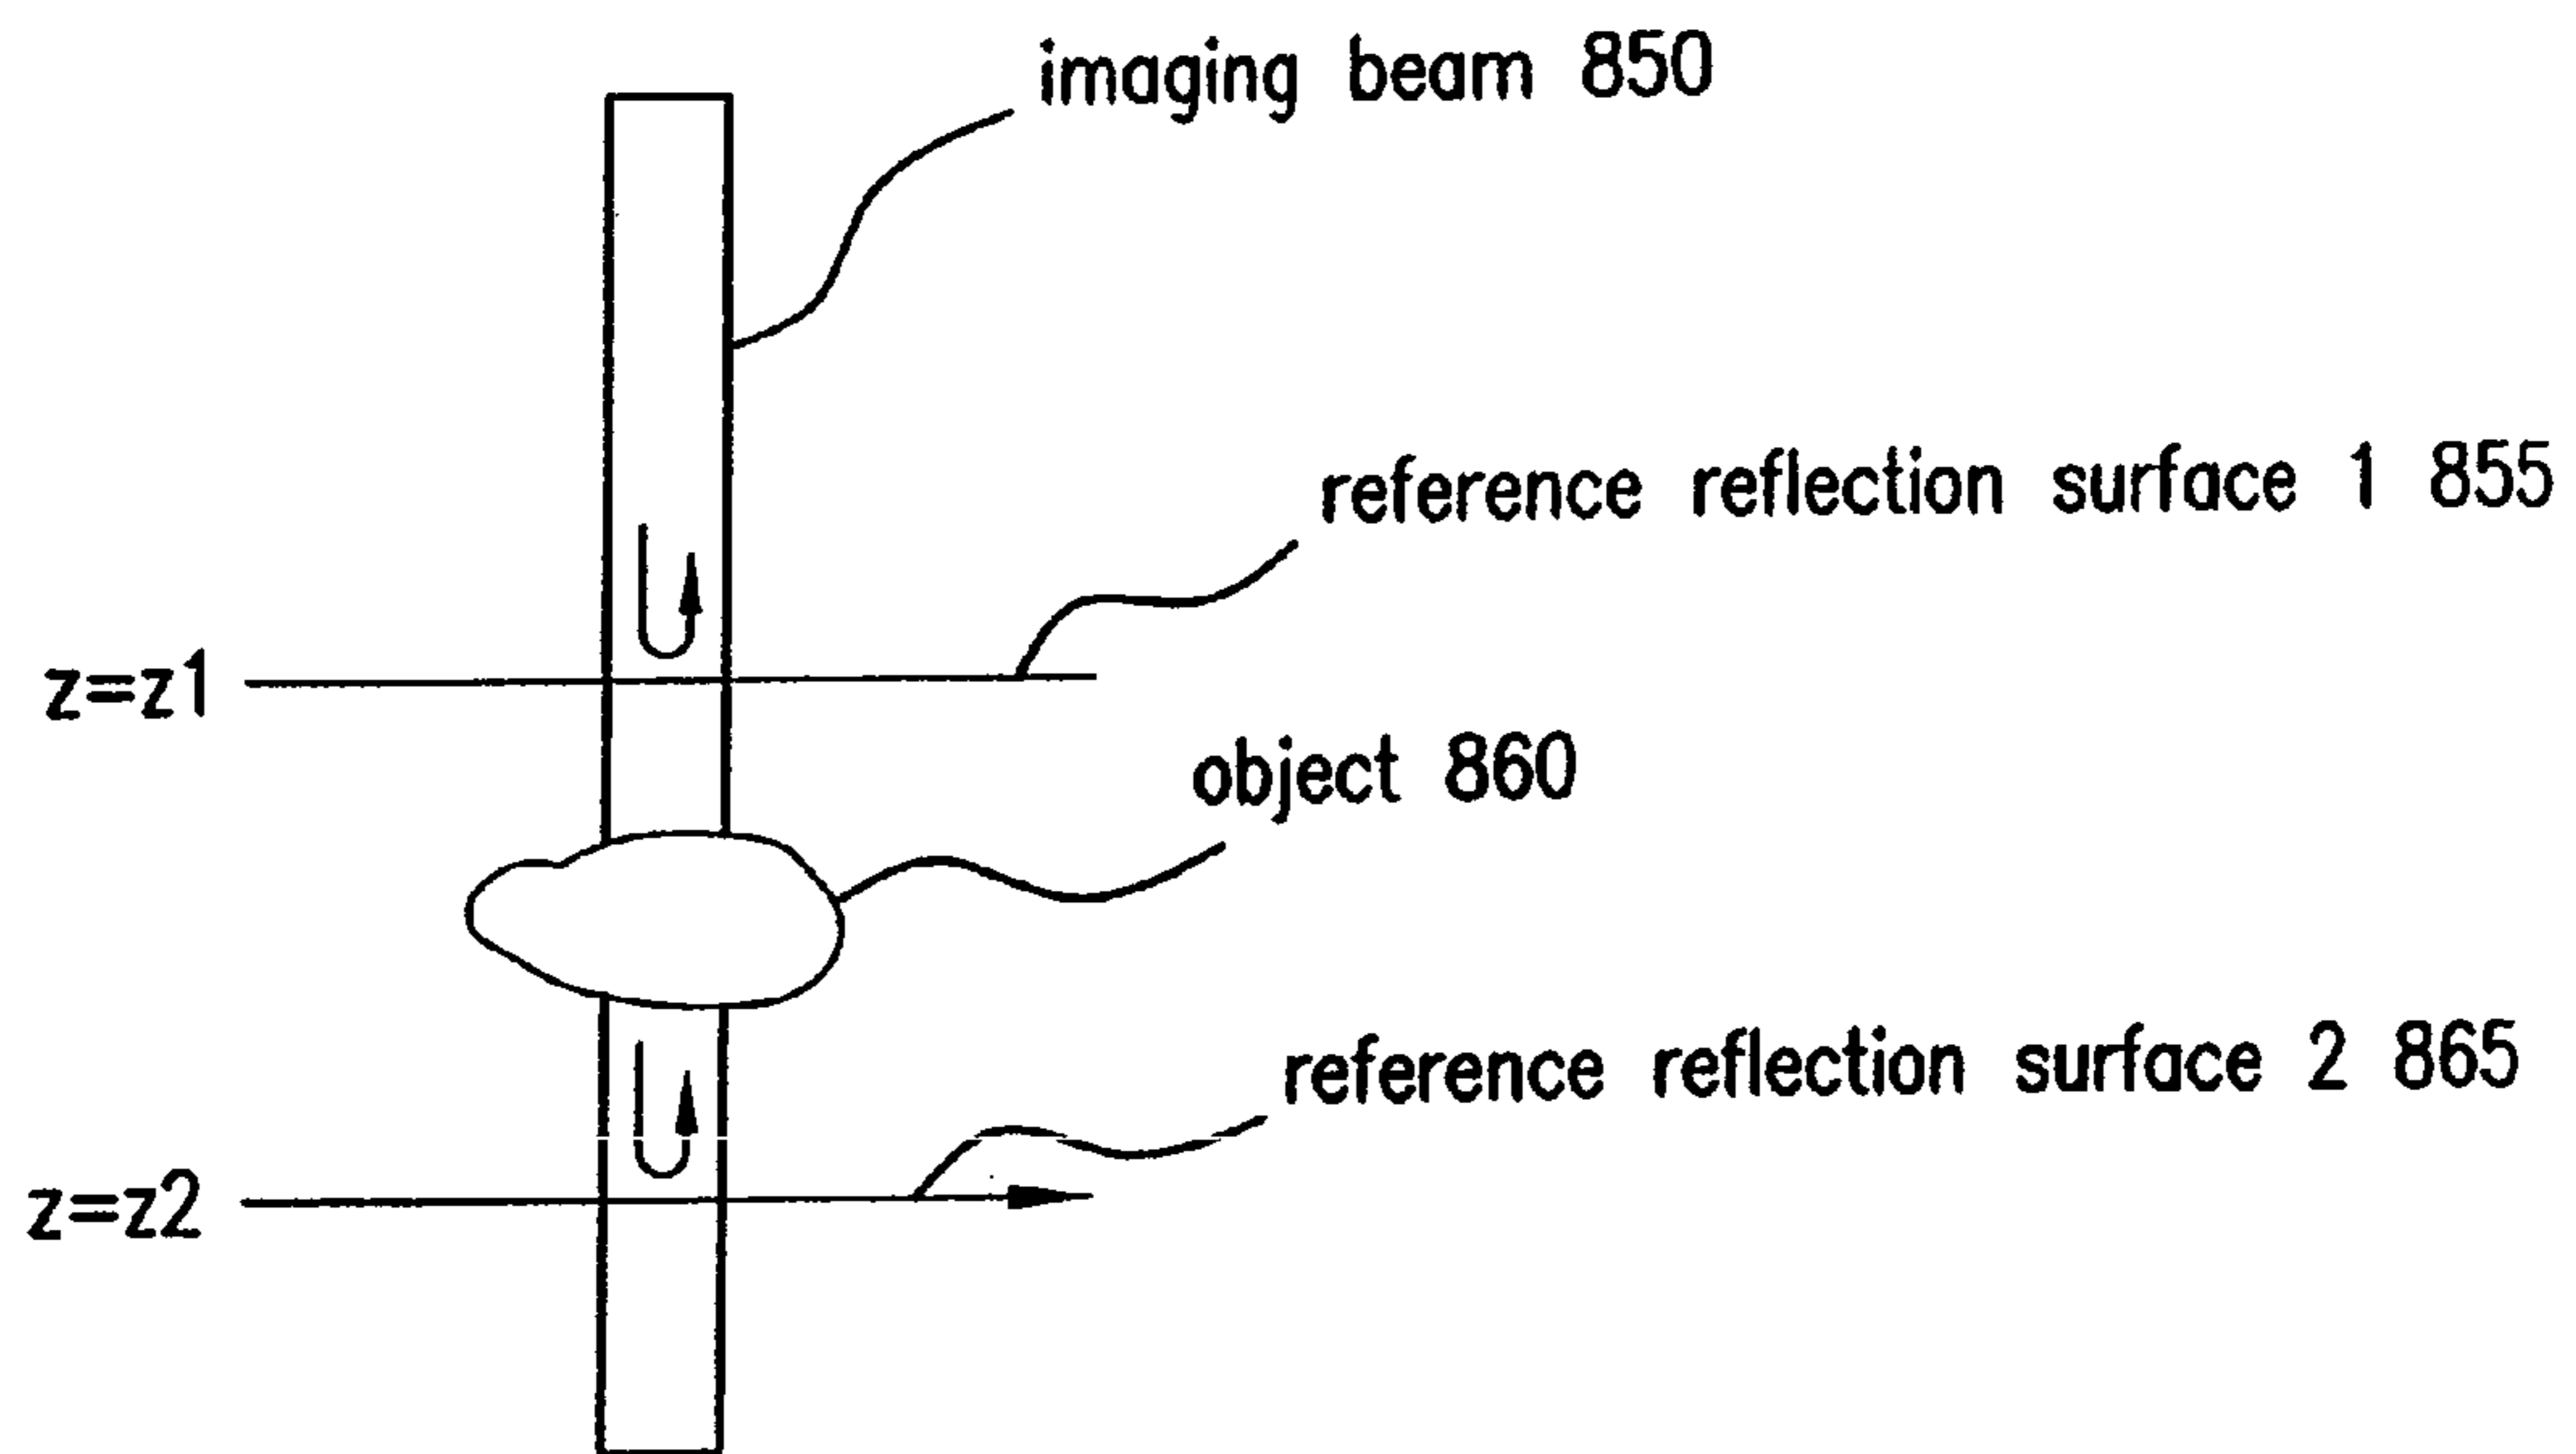

beam translation →

FIG. 10

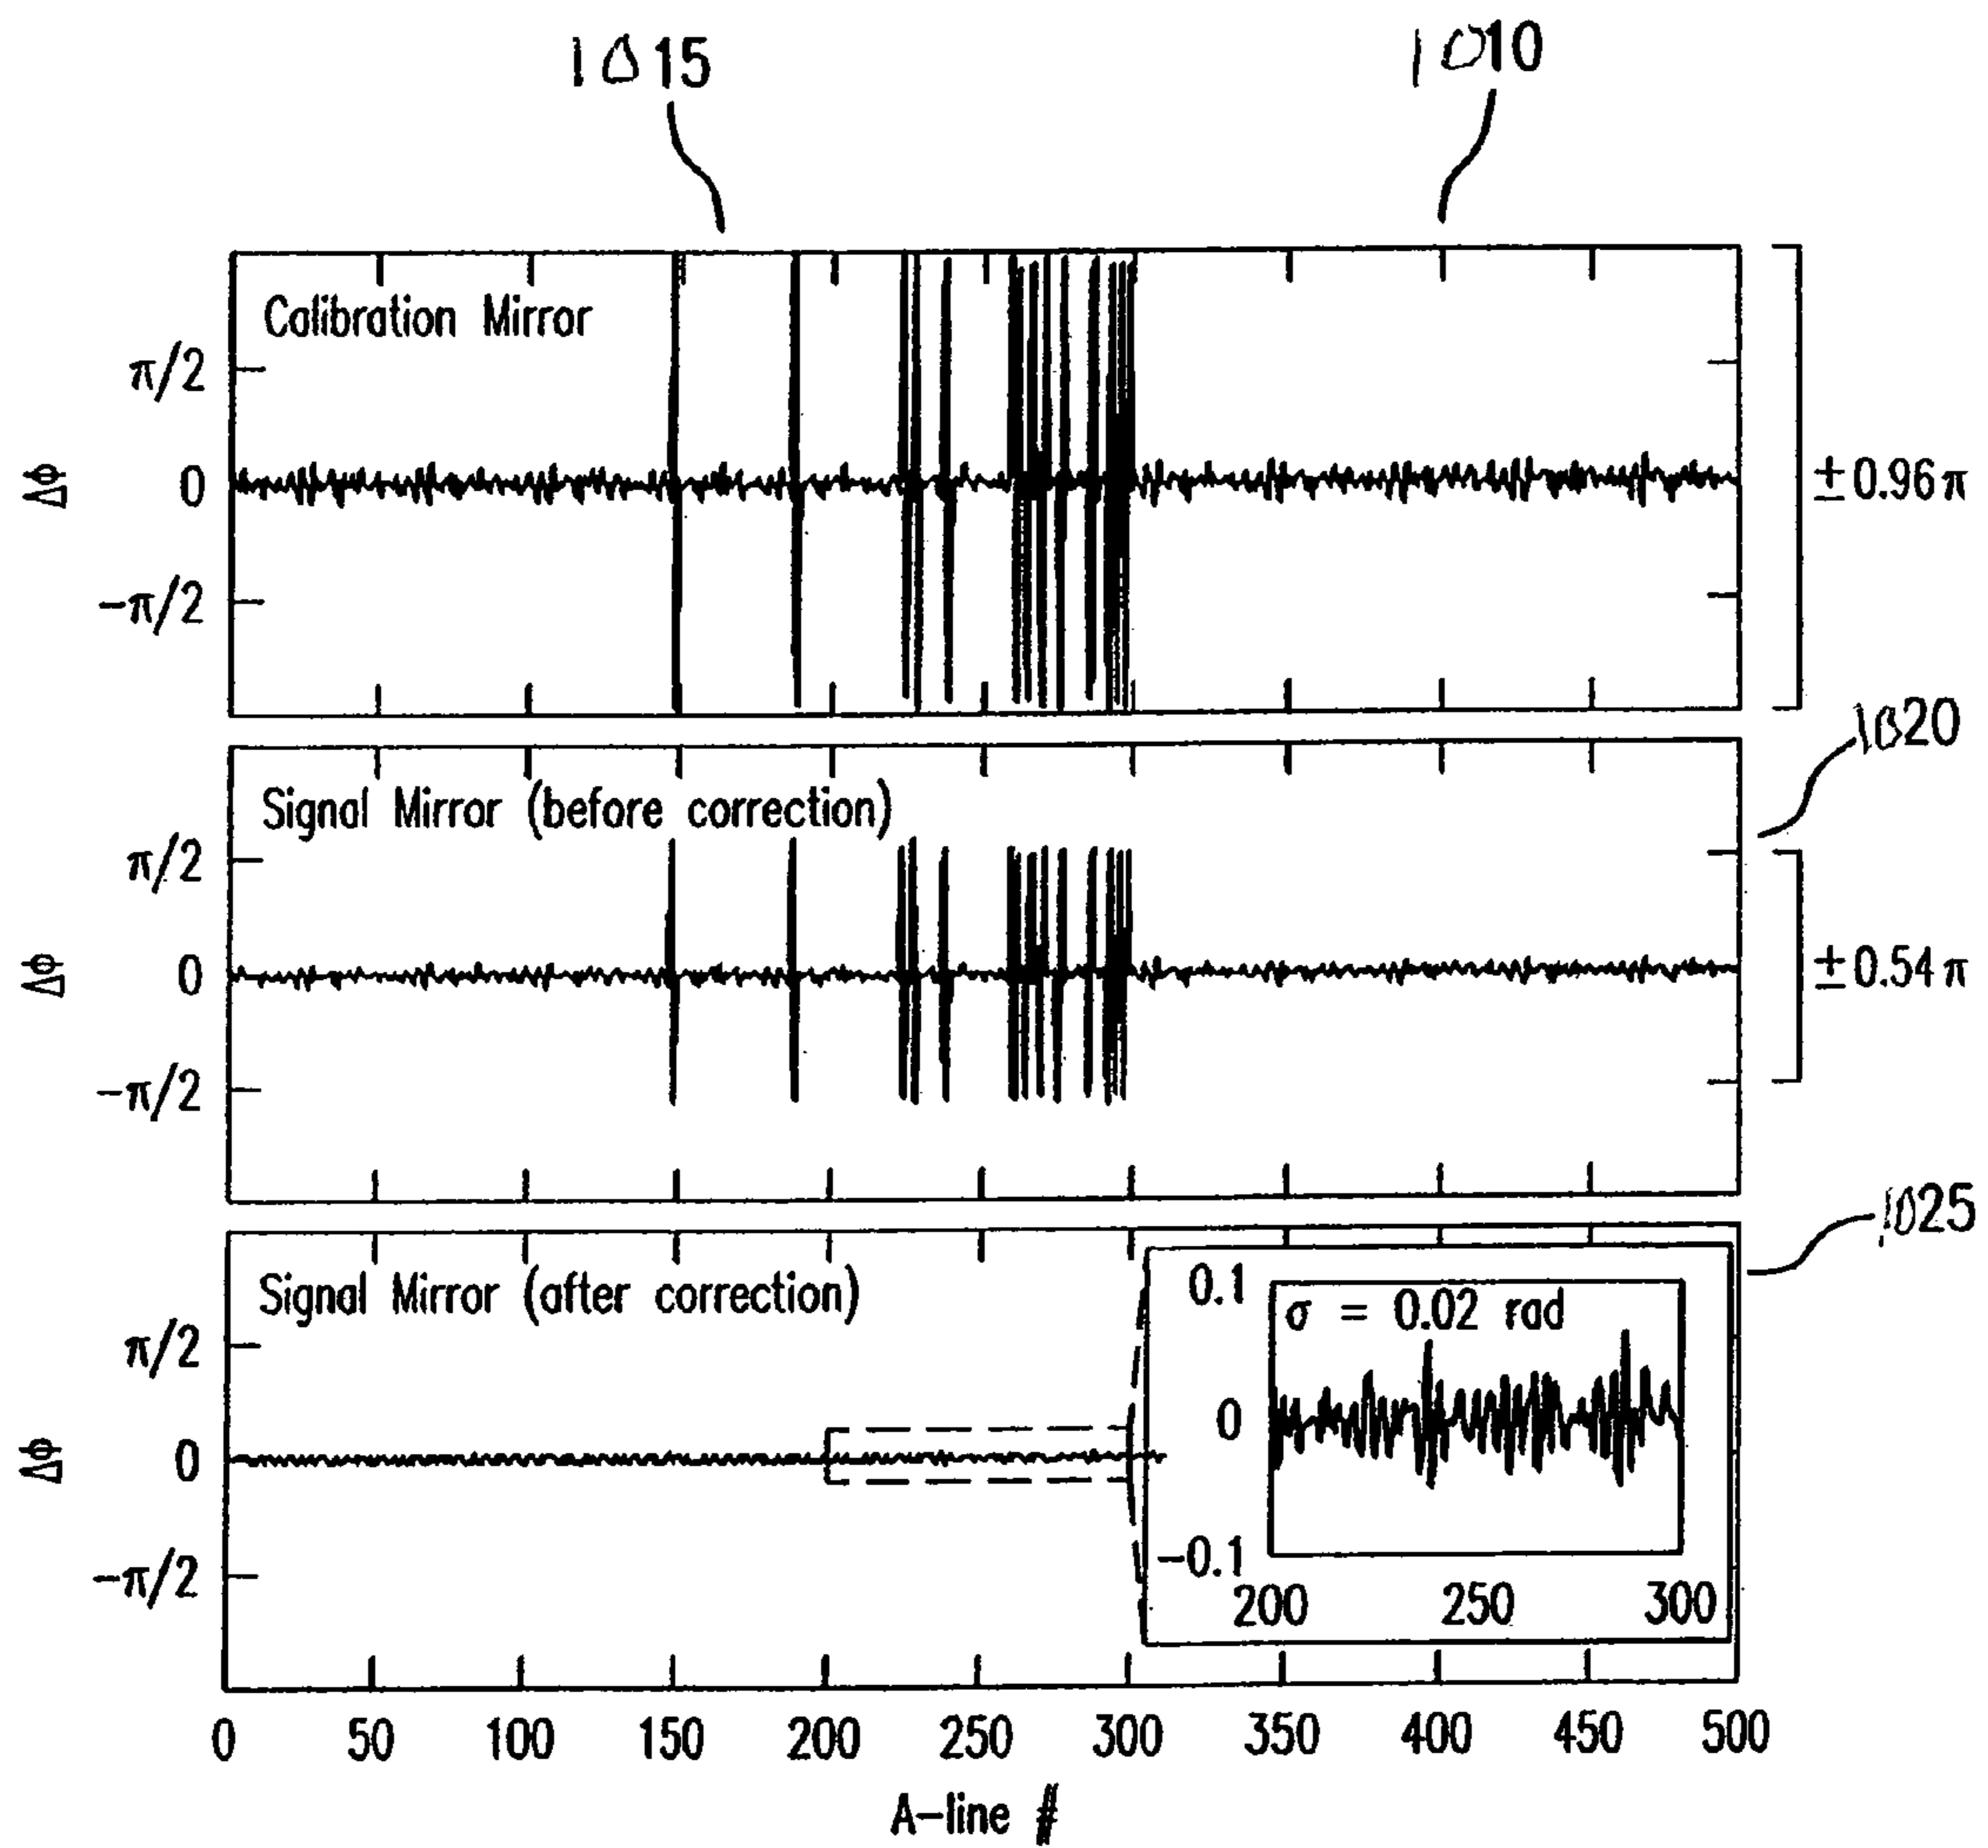


FIG. 11

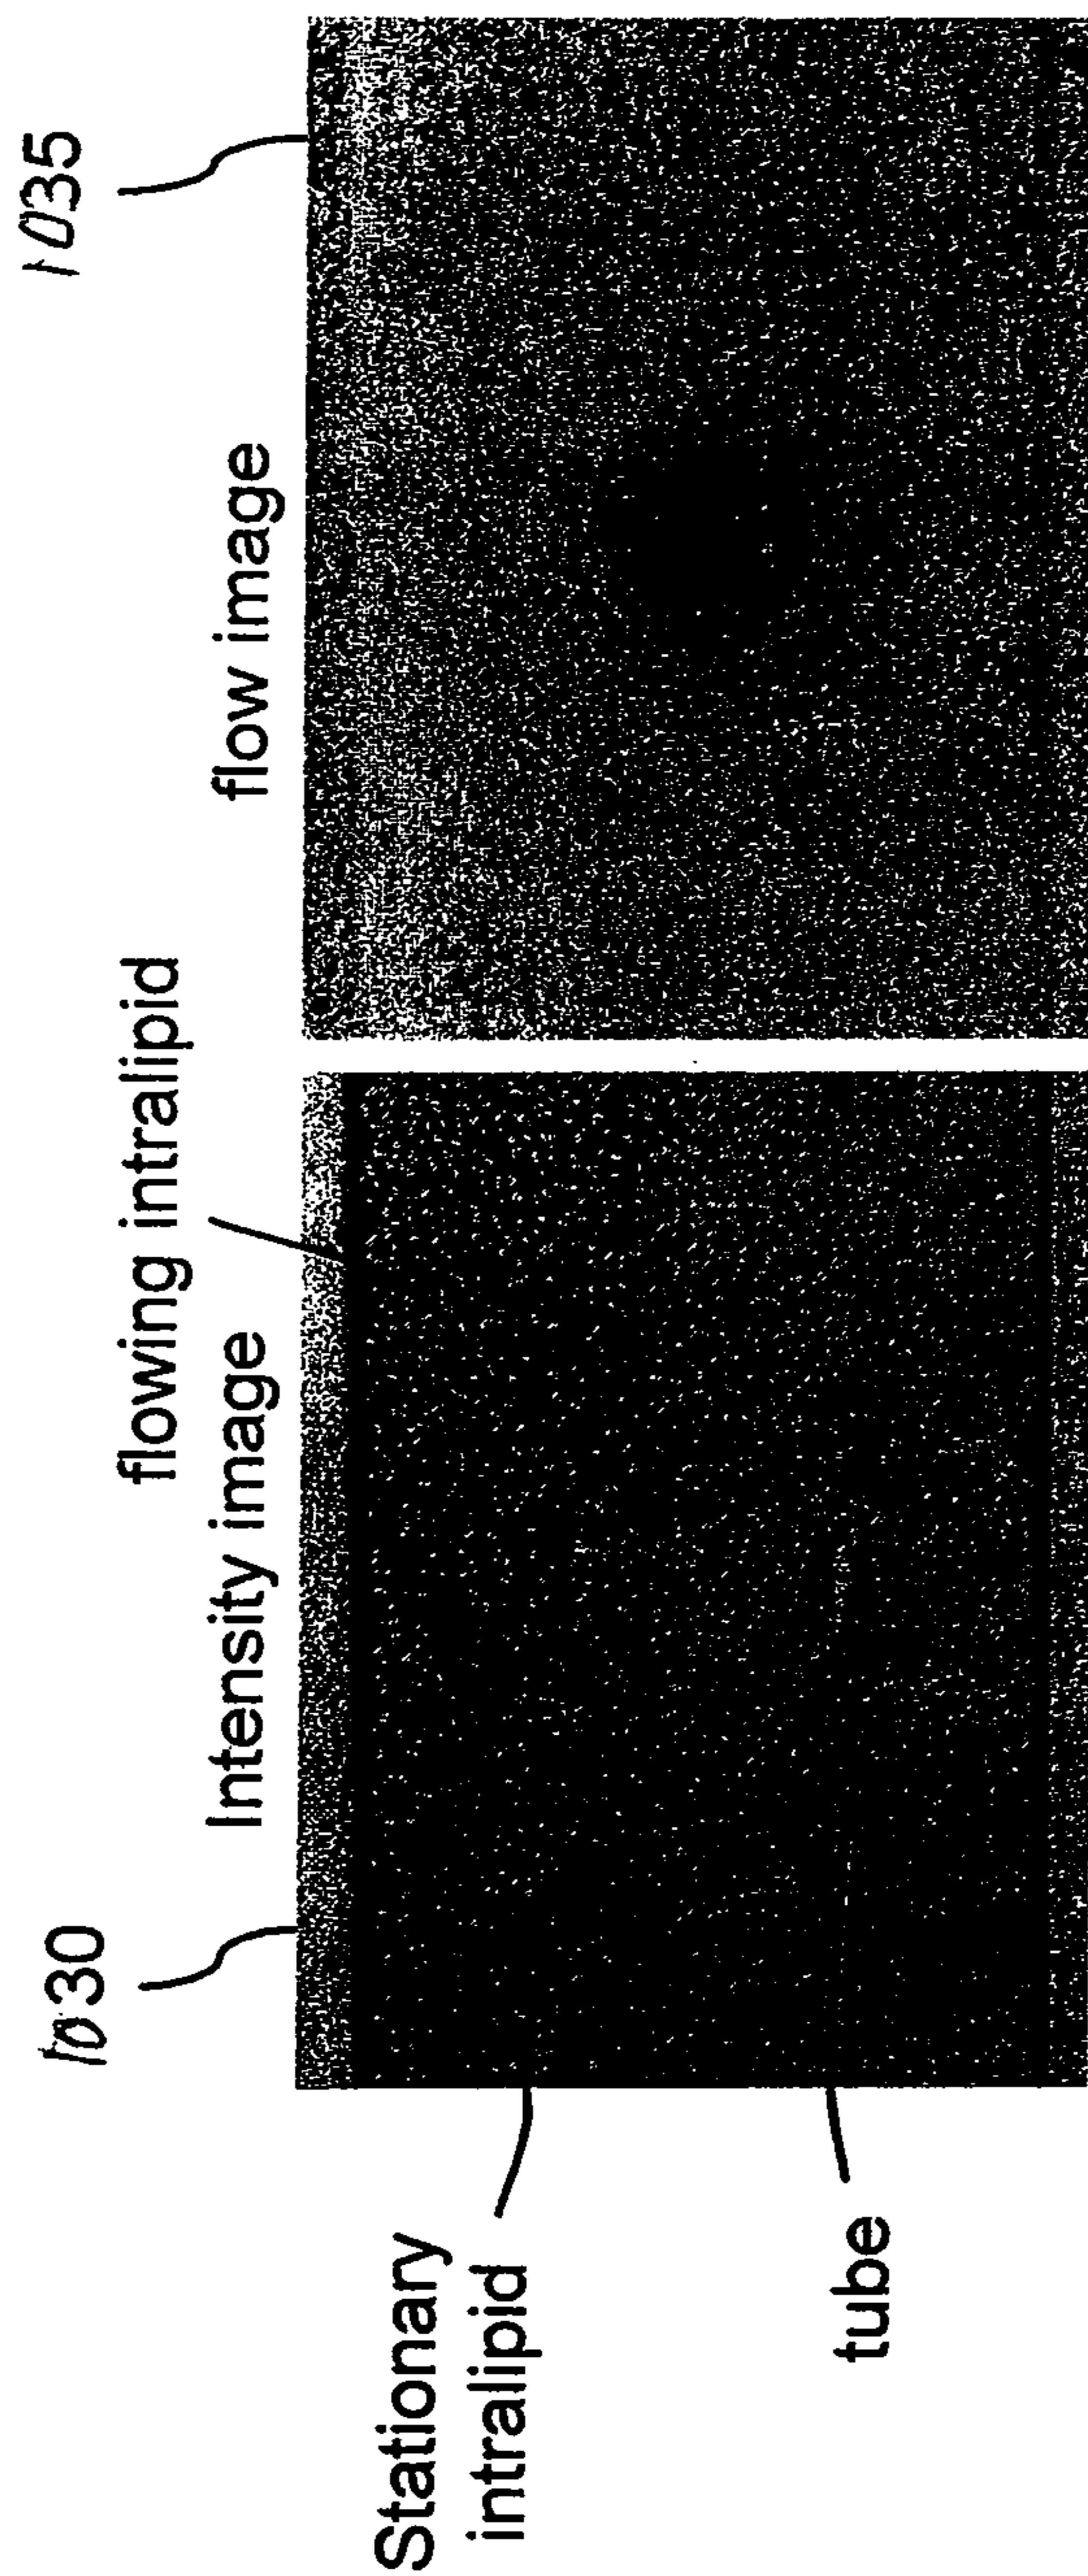


FIG.12

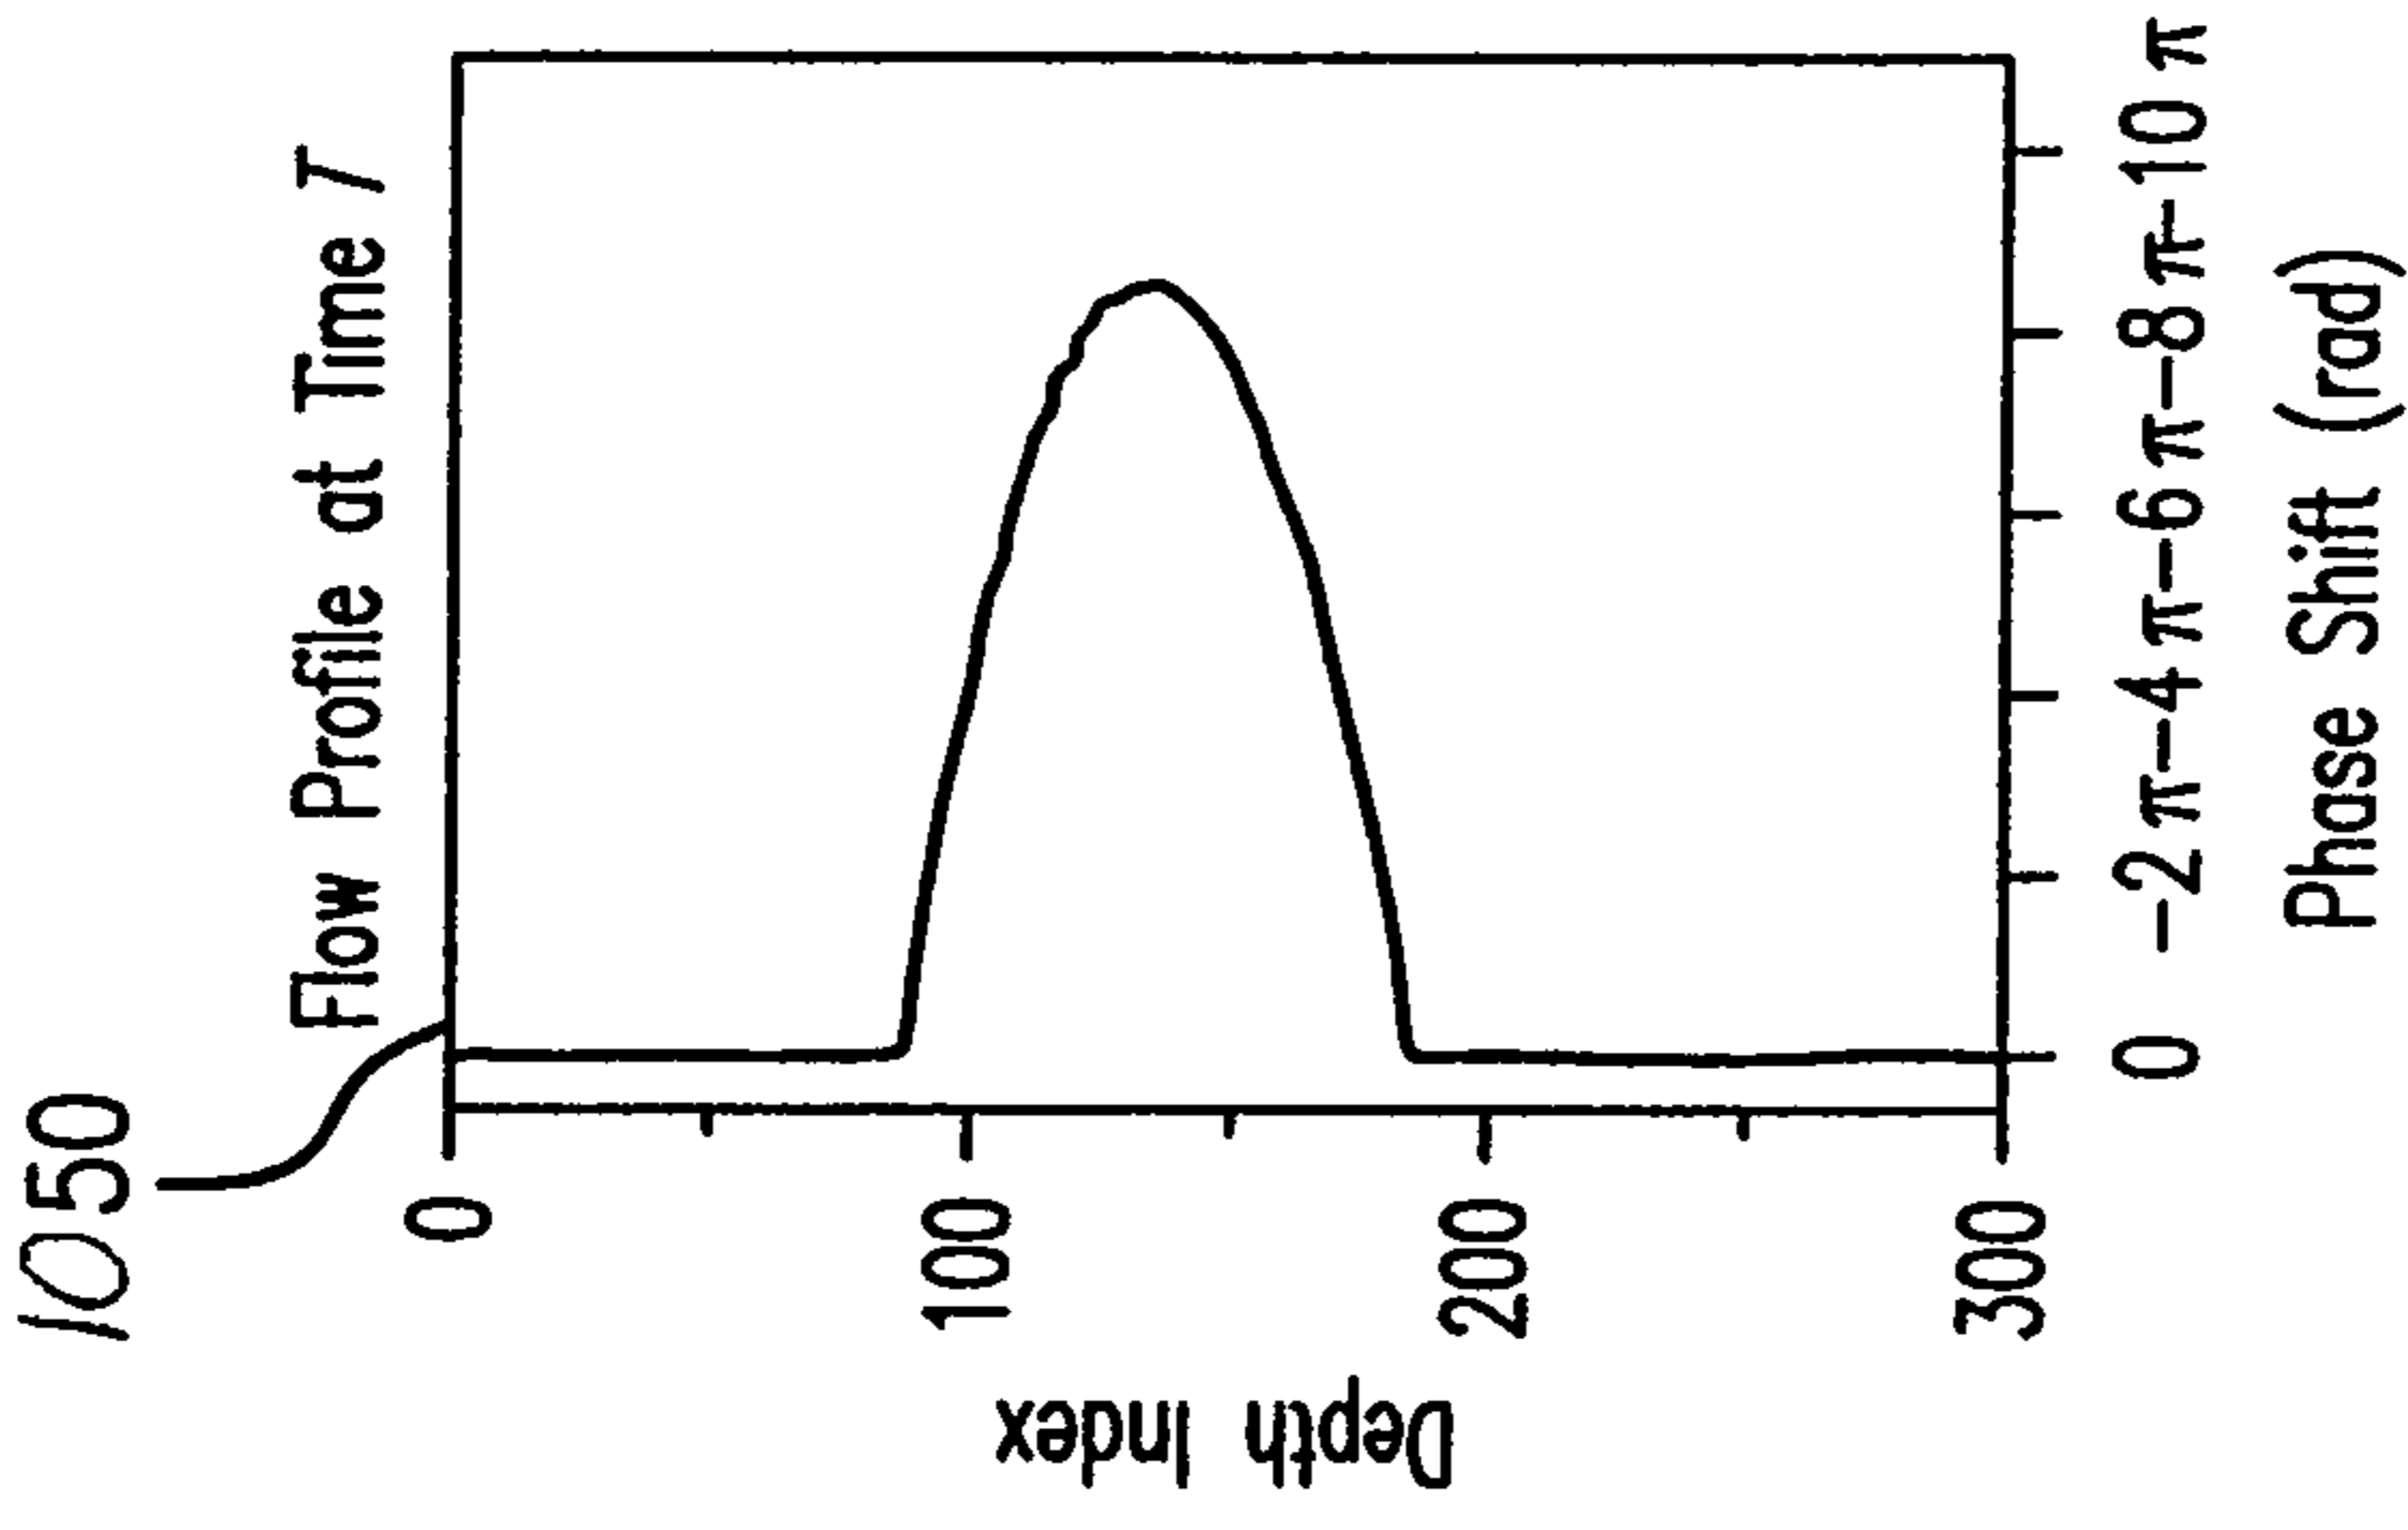


FIG.13C

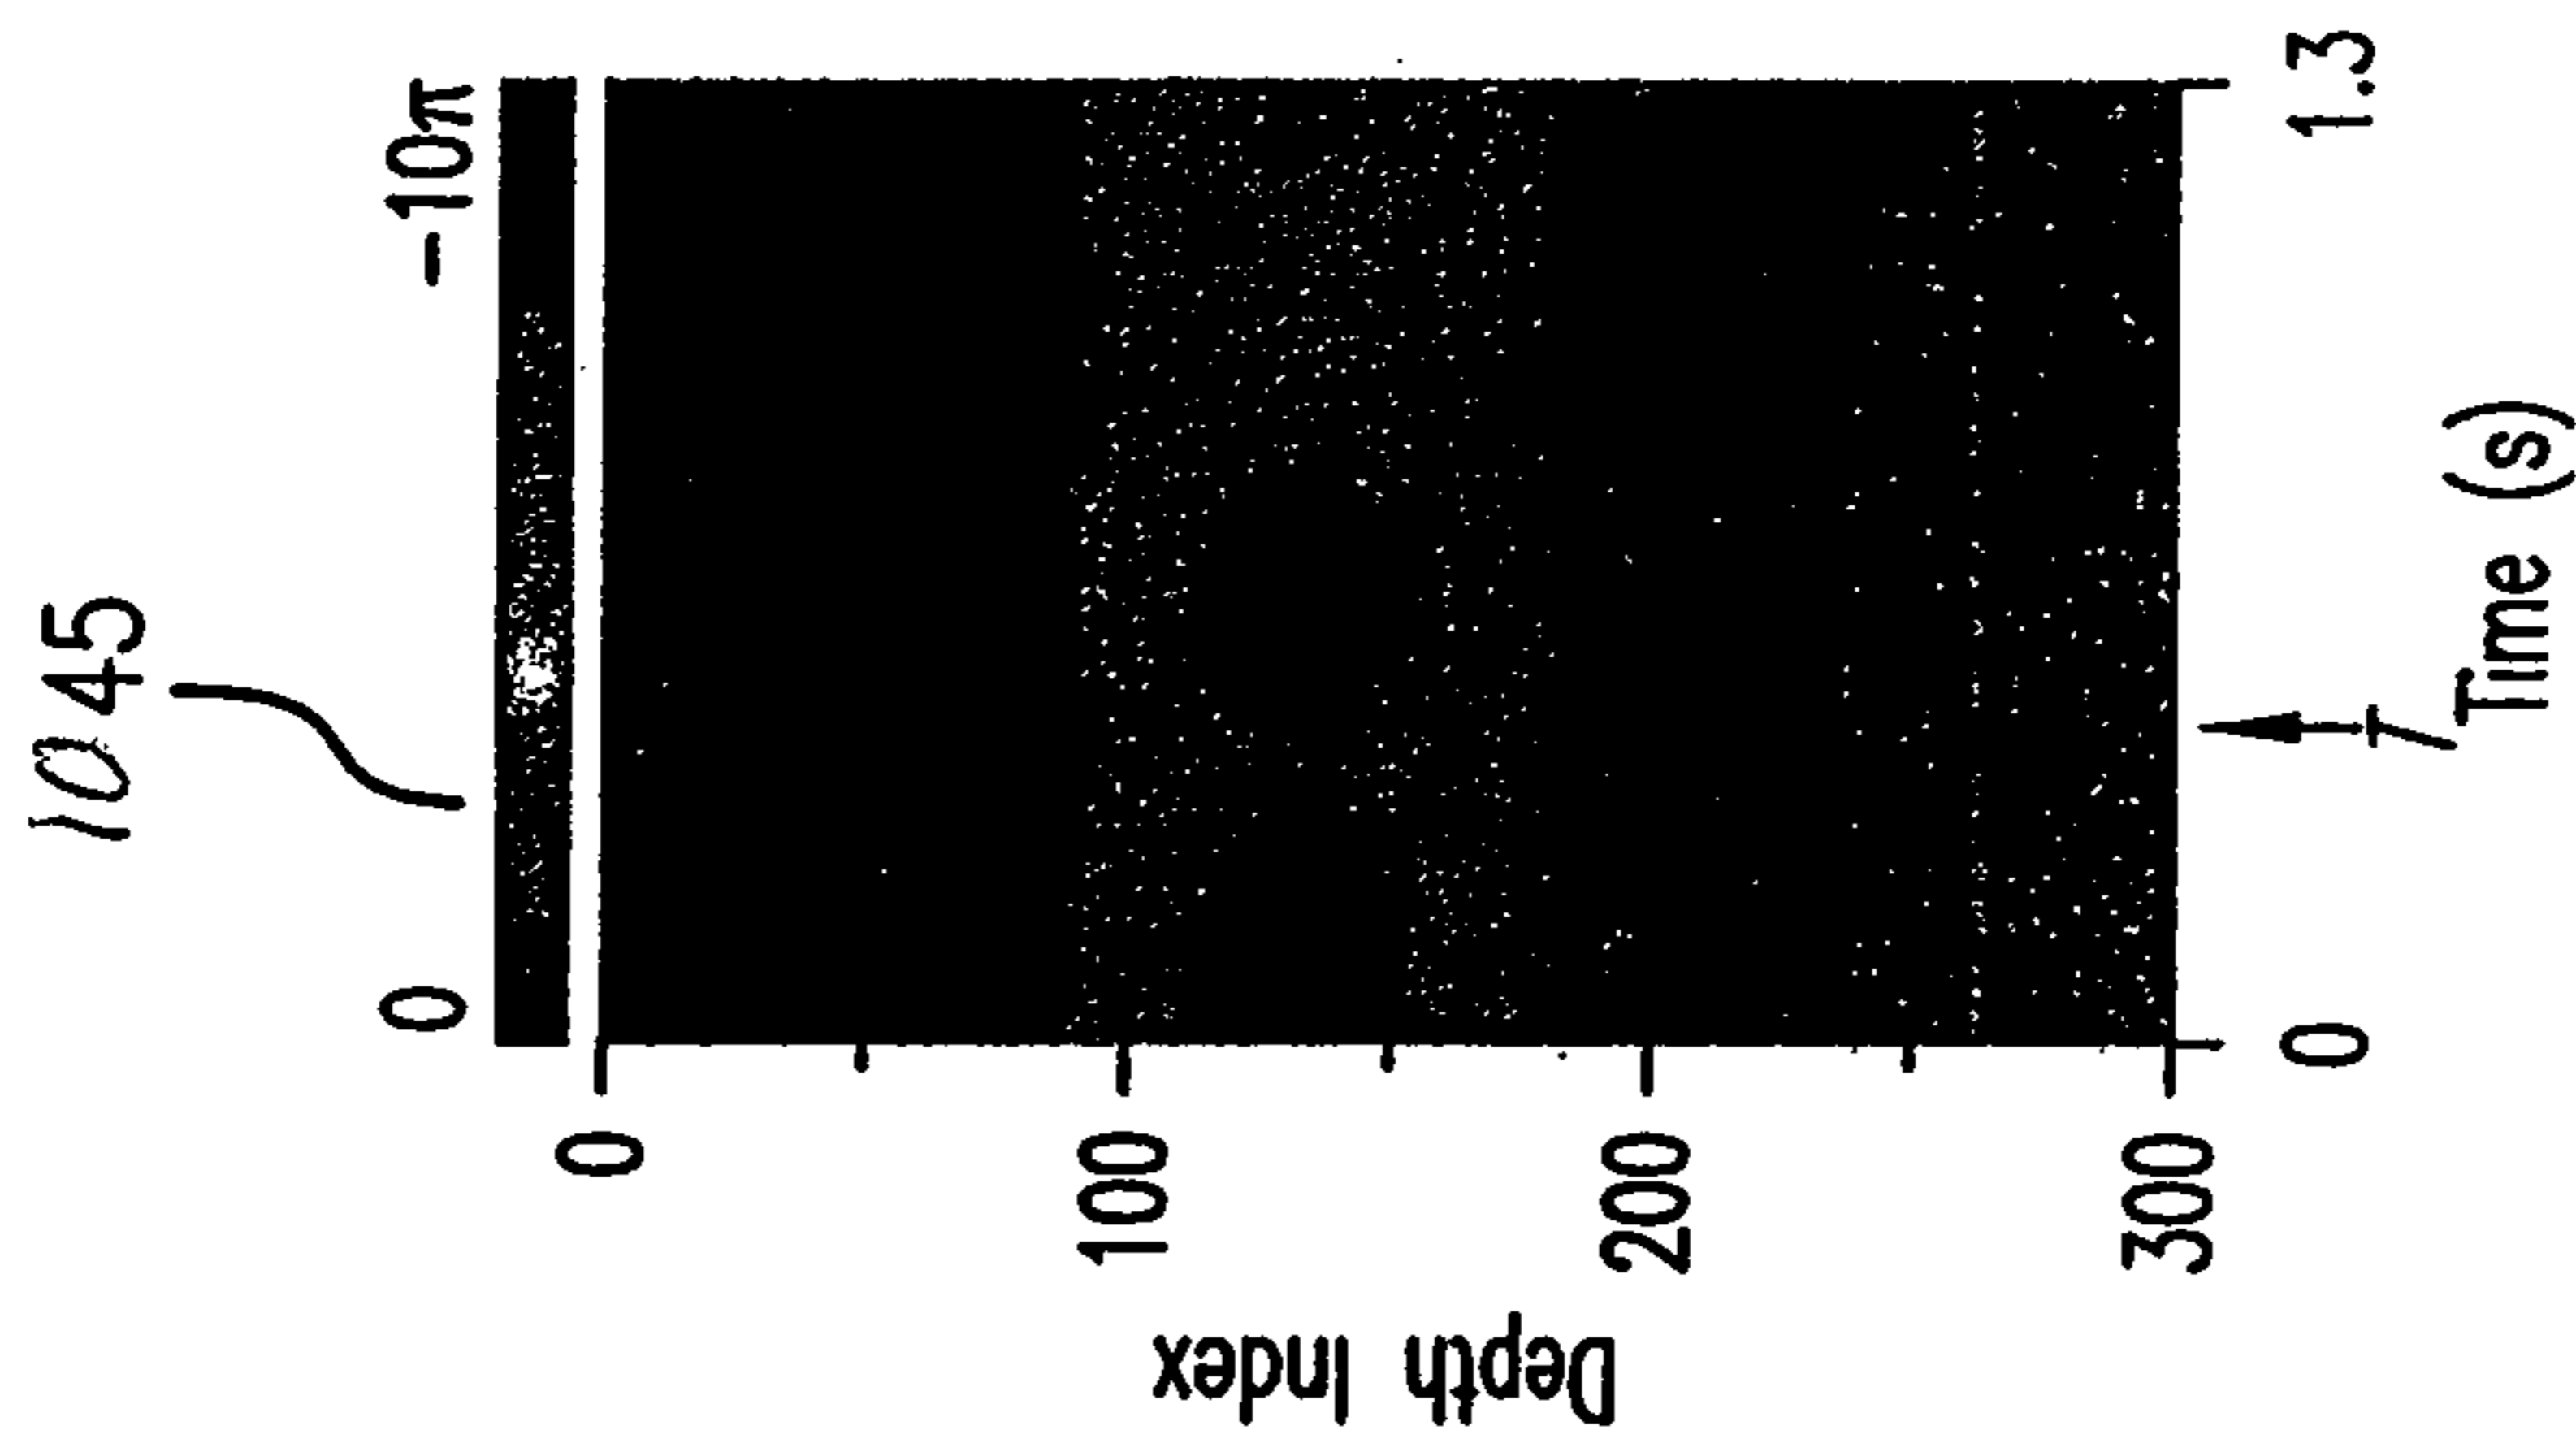


FIG.13B

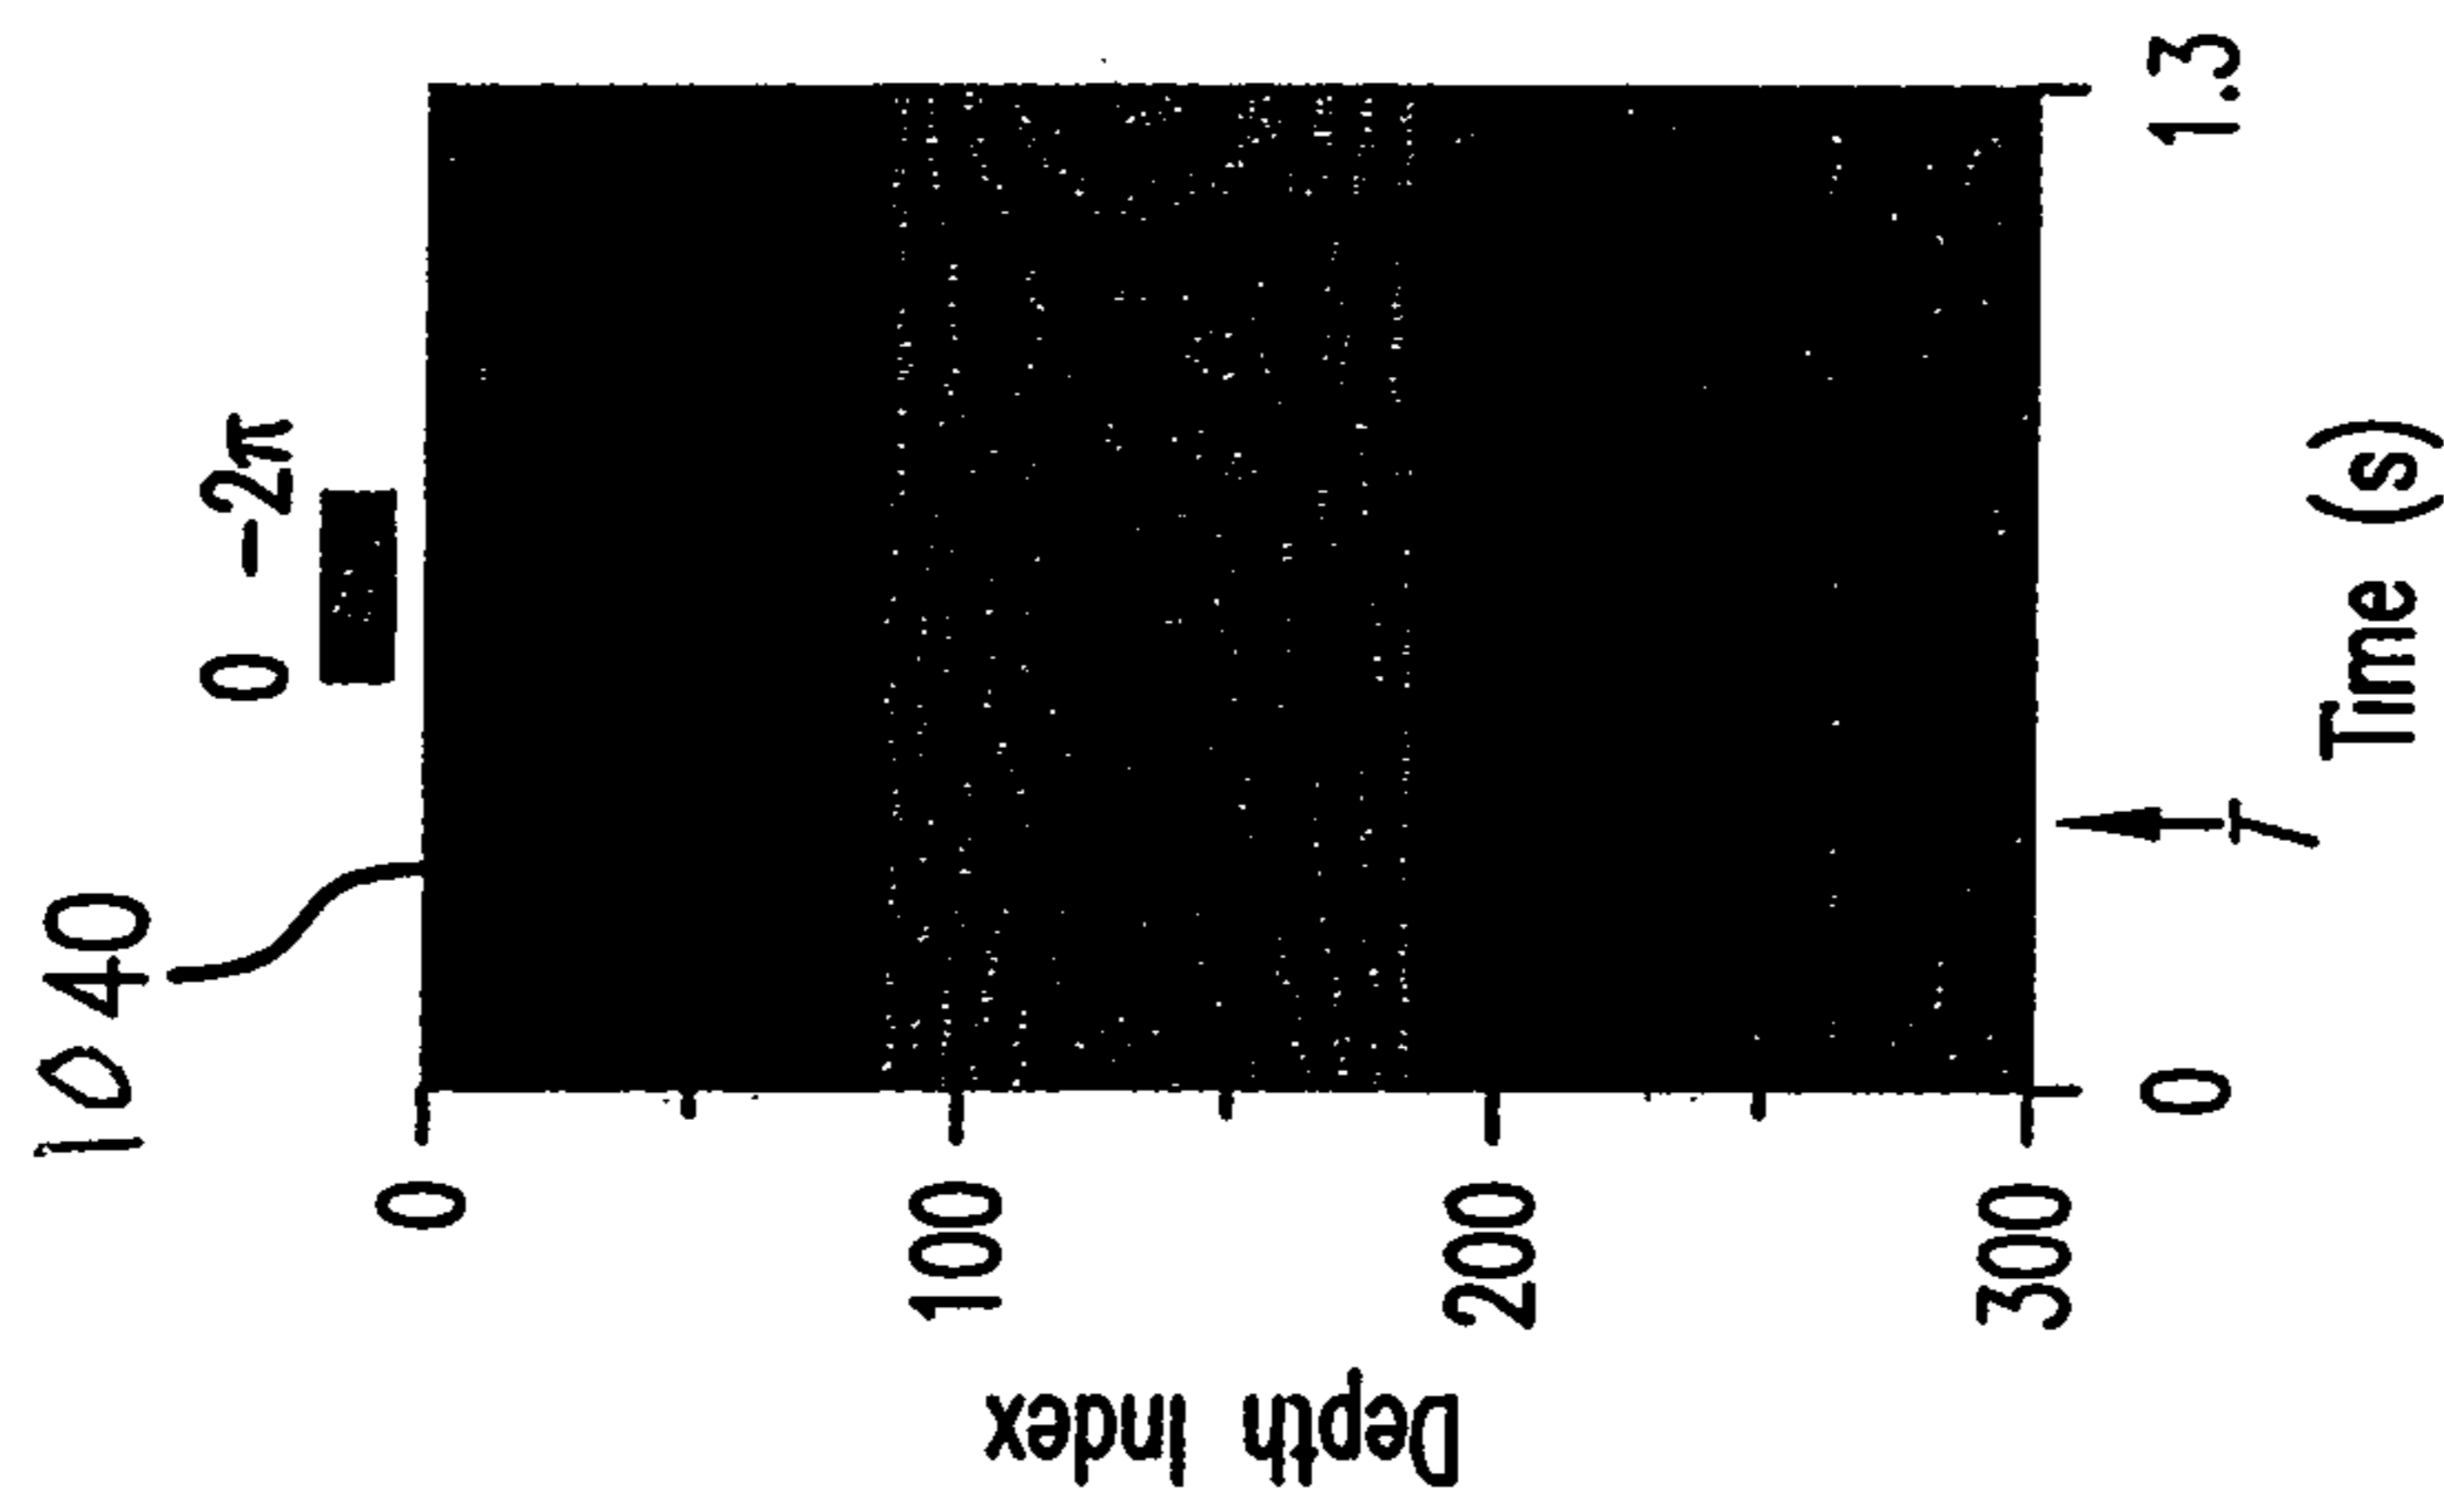


FIG.13A

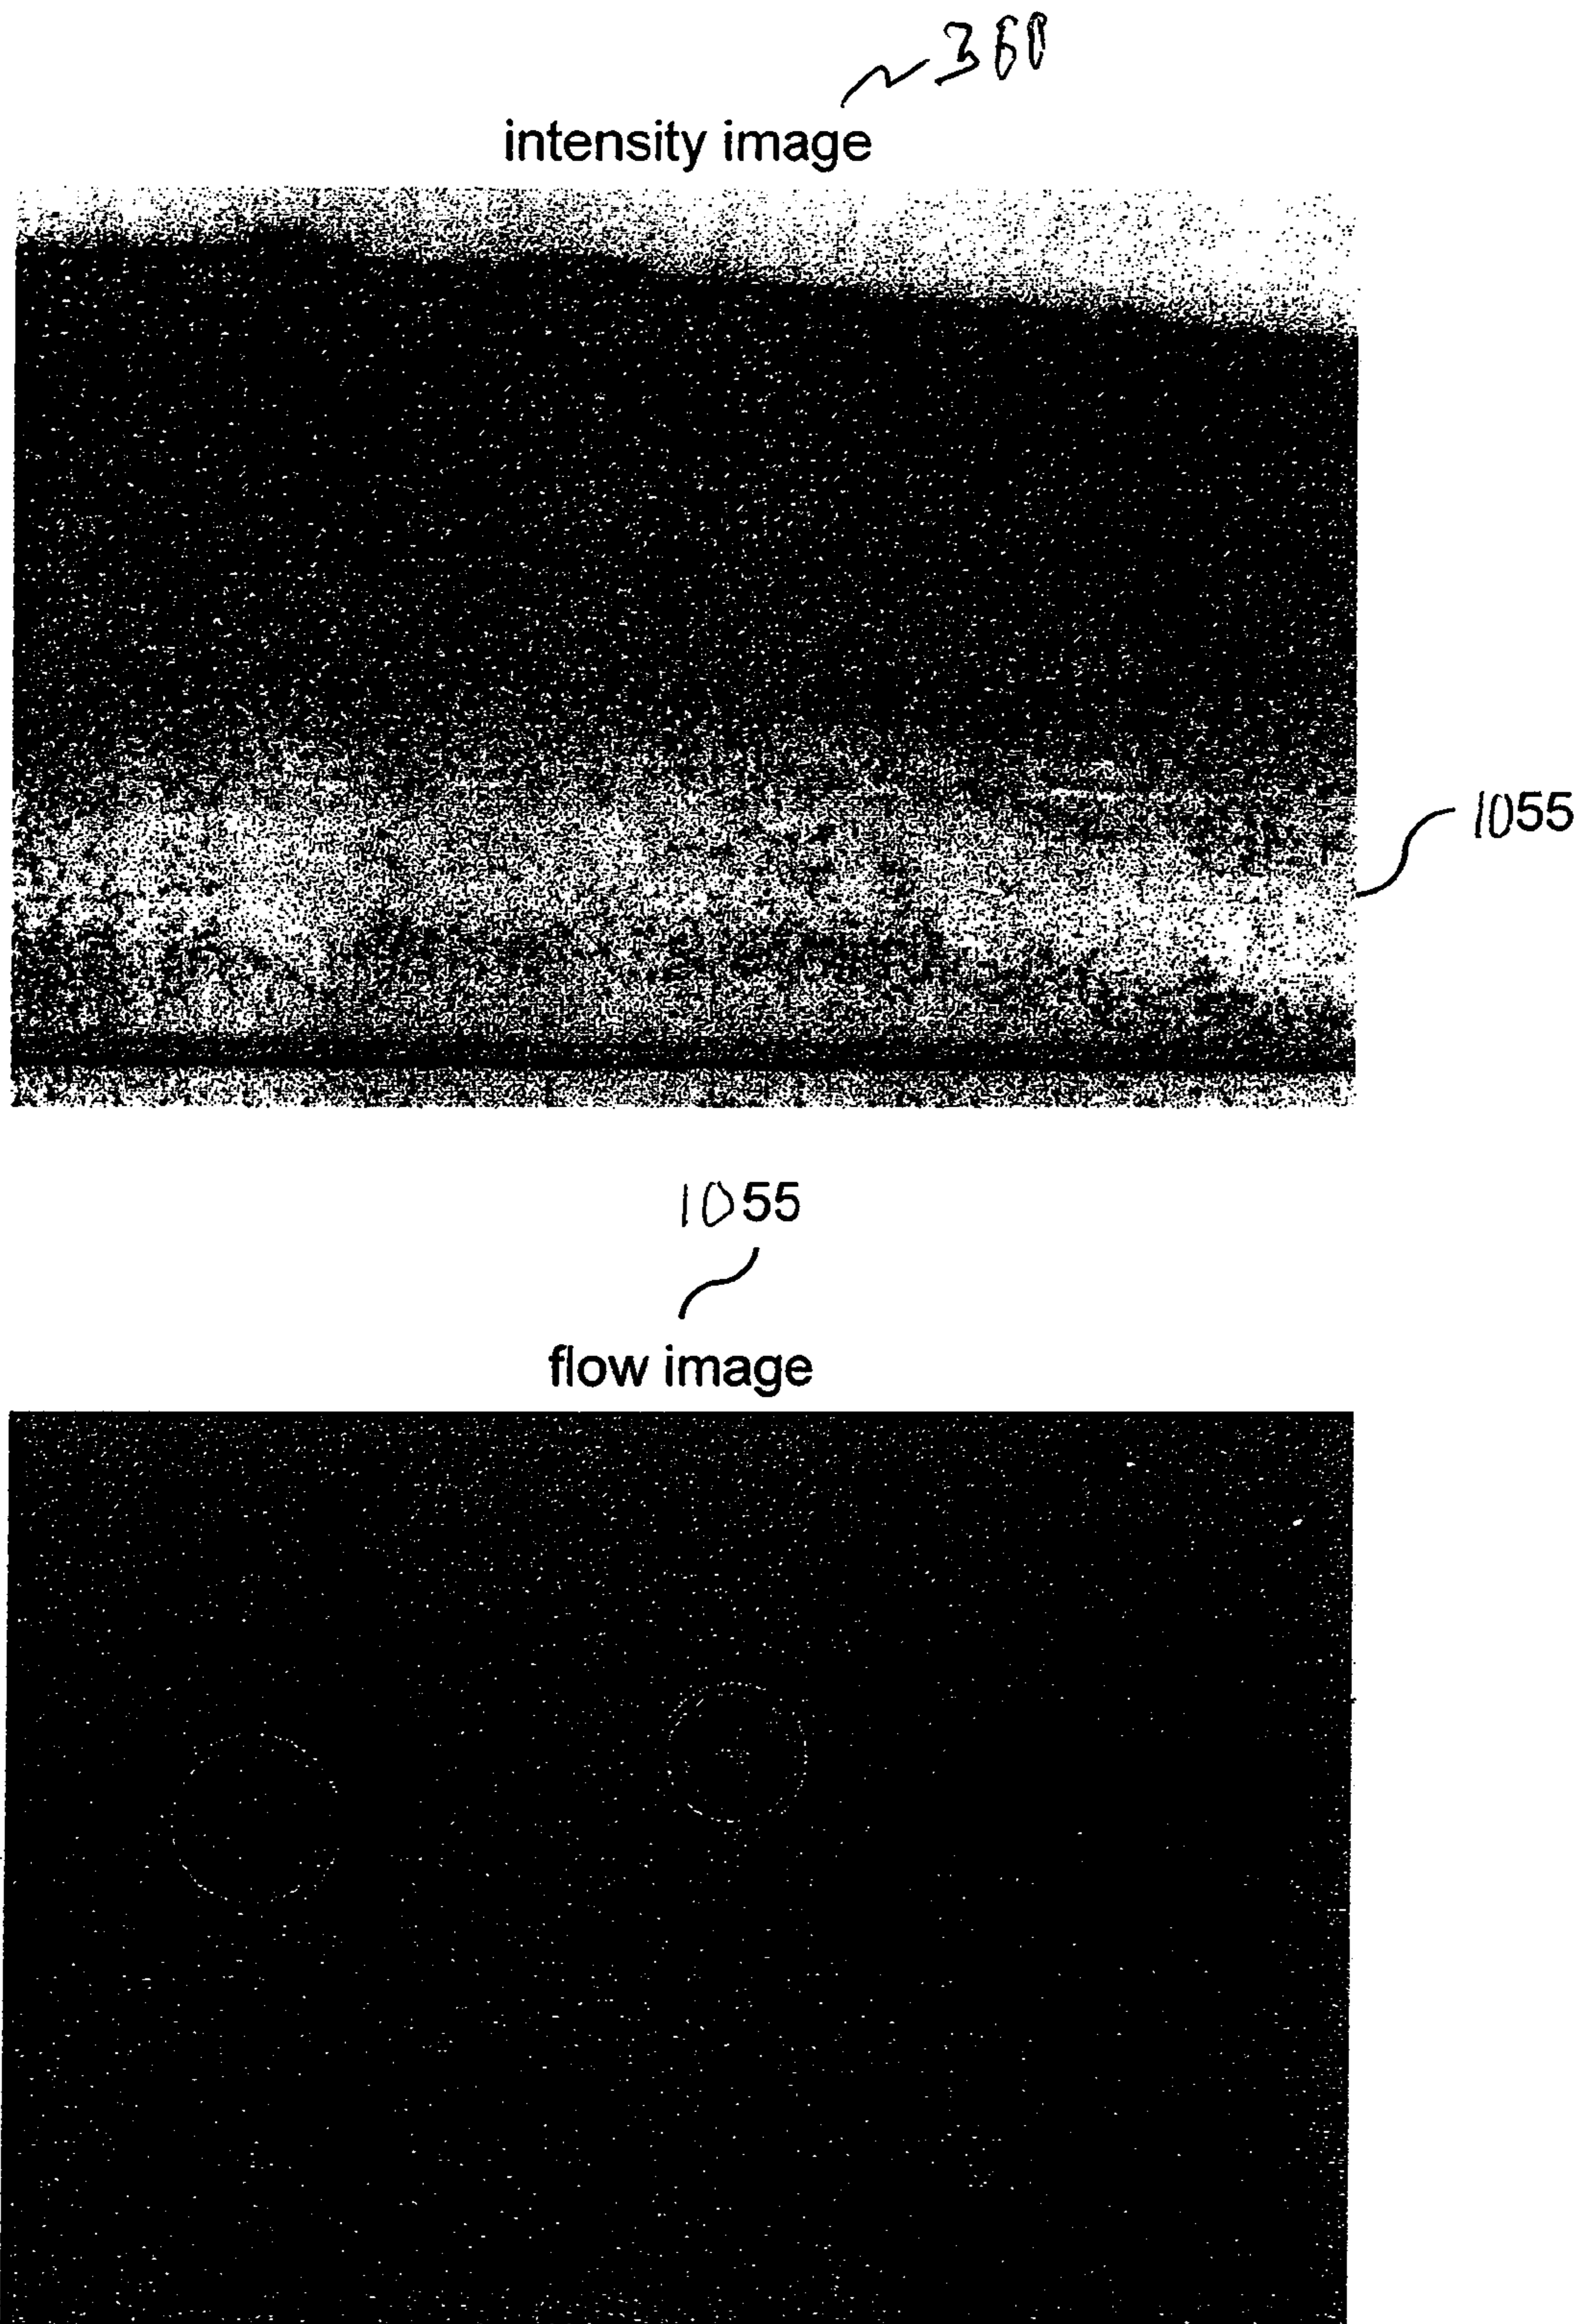


FIG. 14

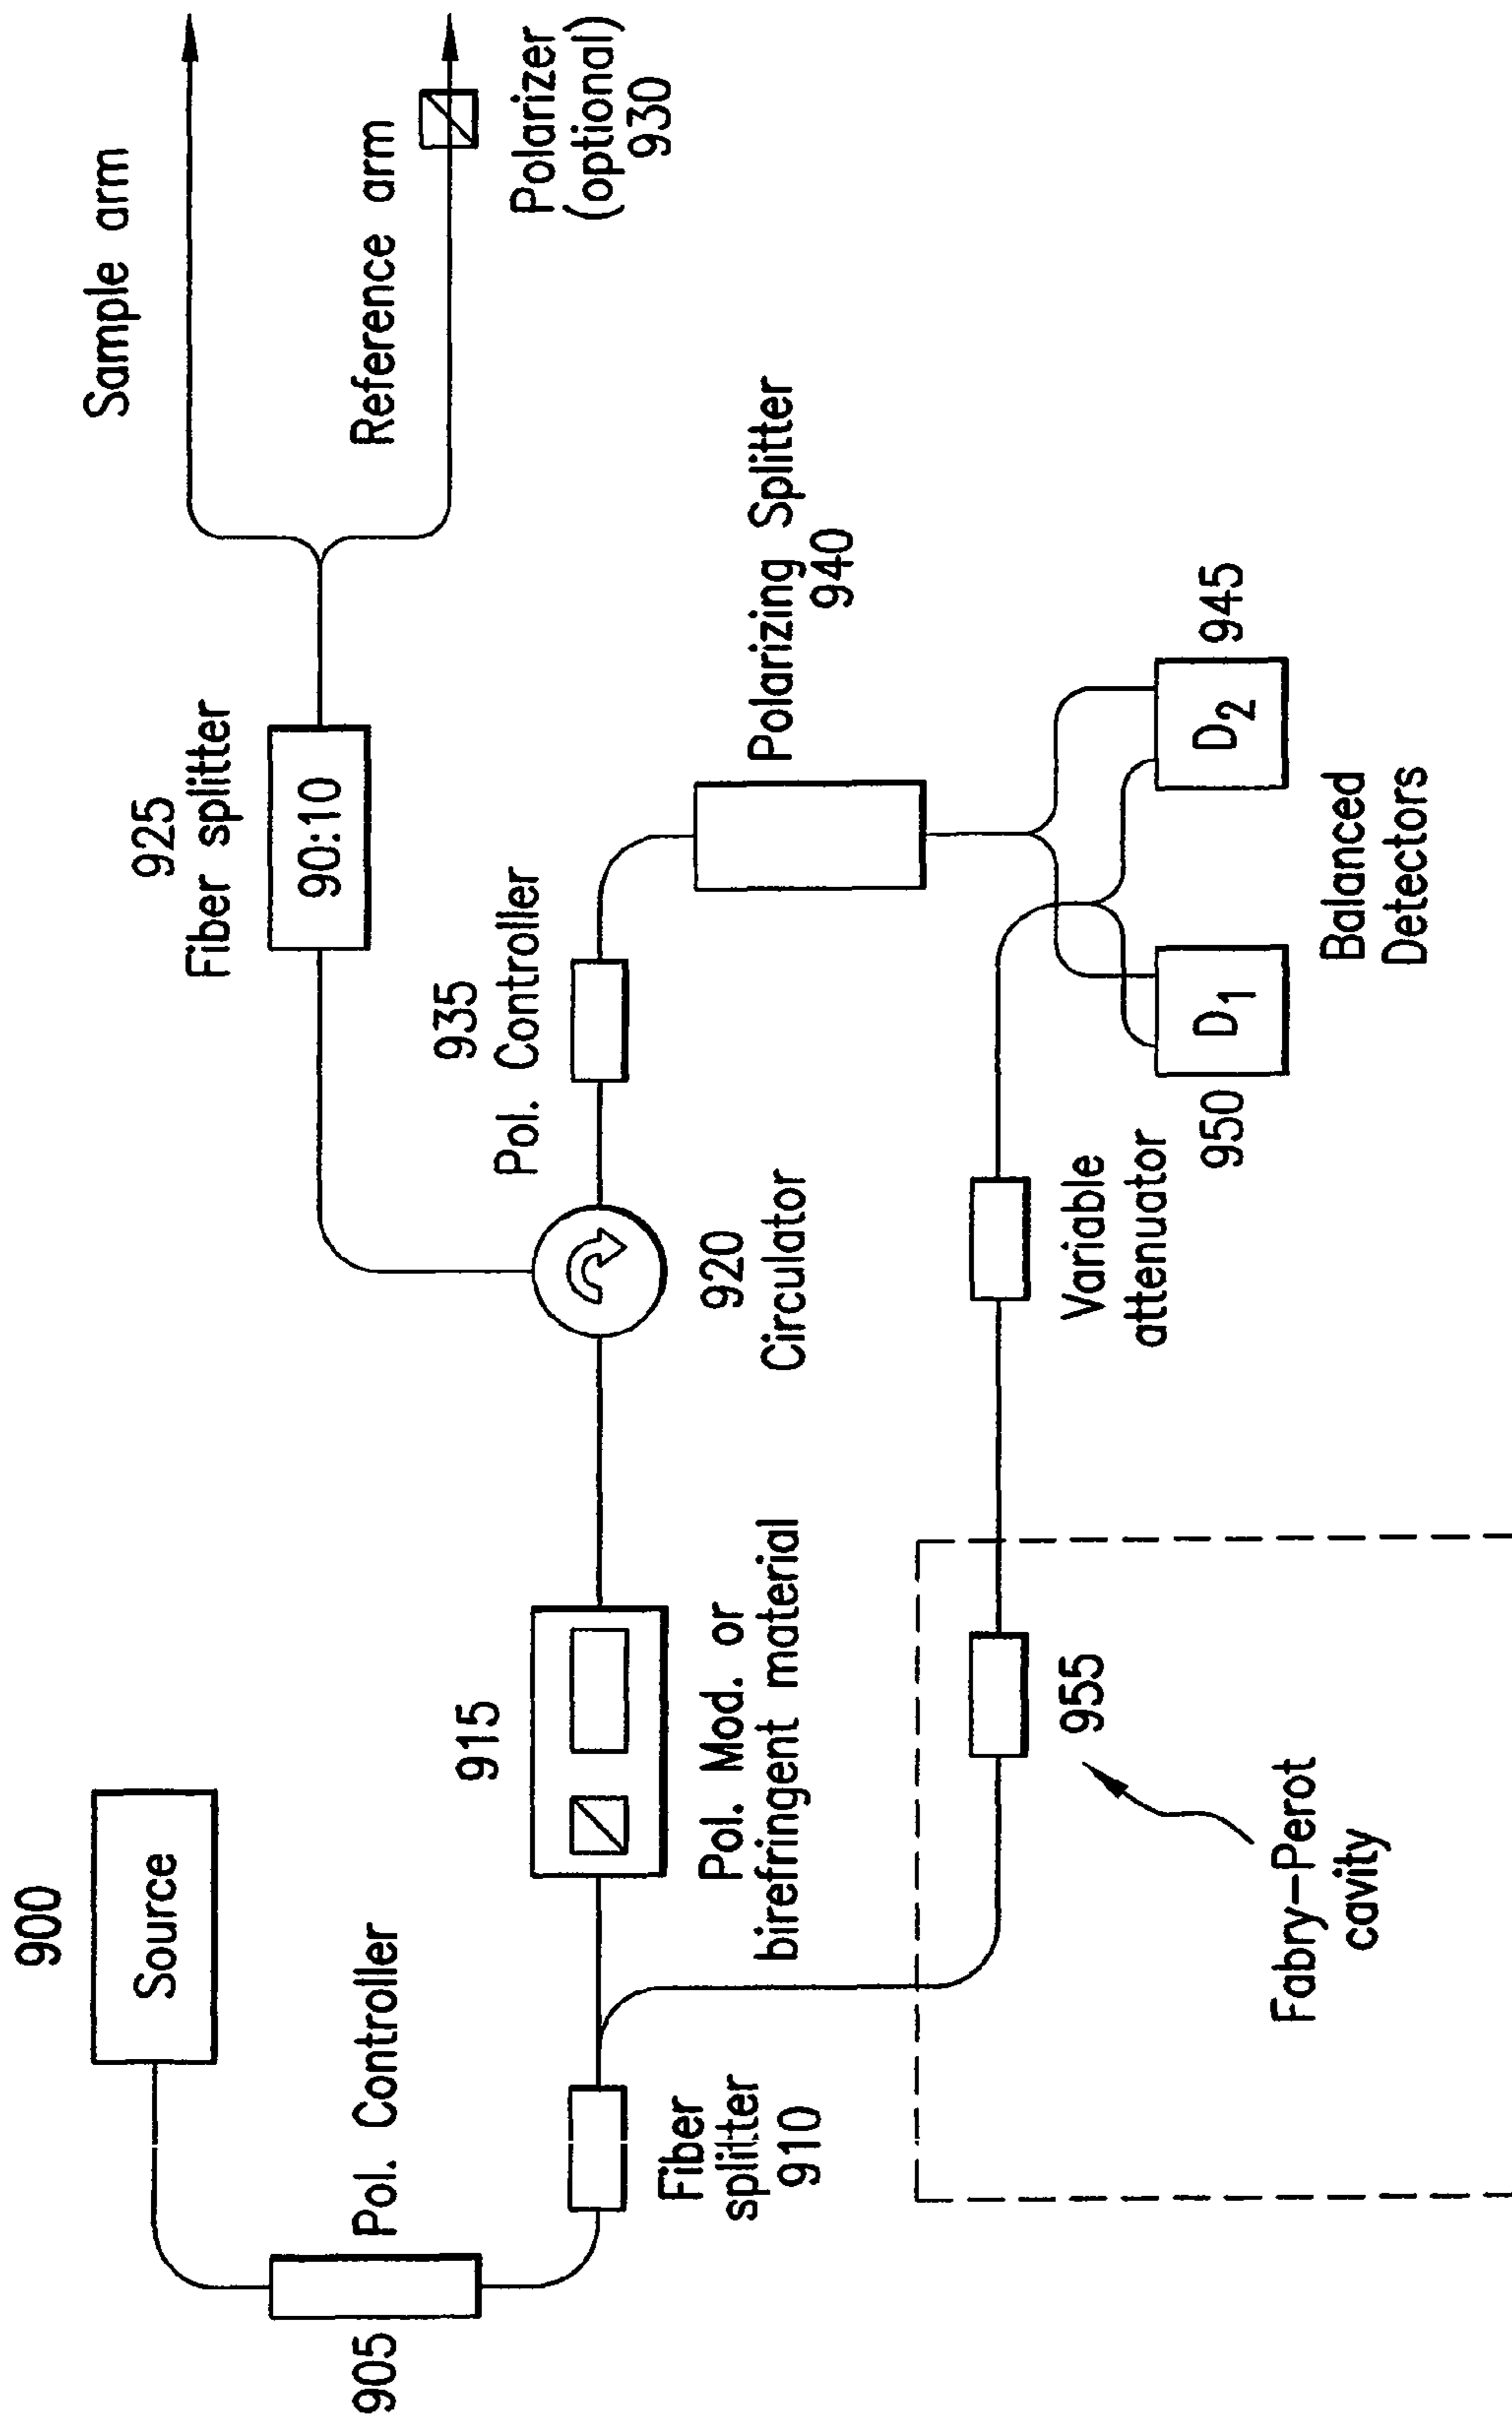


FIG. 15

**APPARATUS, METHOD AND SYSTEM FOR
PERFORMING PHASE-RESOLVED OPTICAL
FREQUENCY DOMAIN IMAGING**

CROSS-REFERENCE TO RELATED
APPLICATION(S)

This application is based upon and claims the benefit of priority from U.S. patent application Ser. No. 60/686,790, filed Jun. 1, 2005, the entire disclosure of which is incorporated herein by reference.

STATEMENT REGARDING FEDERALLY
SPONSORED RESEARCH

The research leading to the present invention was supported, at least in part, by National Institute of Health, Grant numbers R33 CA110130 and R01 HL70039. Thus, the U.S. government may have certain rights in the invention.

FIELD OF THE INVENTION

The present invention relates to apparatus, method and system for imaging at least a portion of a sample in an optical frequency domain, and more particularly for performing phase-resolved imaging of transparent and turbid samples using optical frequency domain imaging techniques.

BACKGROUND INFORMATION

Optical coherence tomography ("OCT") is an imaging technique that measures the interference between a reference beam of light and a beam reflected back from a sample. A detailed system description of traditional time-domain OCT was first described in Huang et al. "Optical Coherence Tomography," *Science* 254, 1178 (1991). Detailed system descriptions for spectral-domain OCT and Optical Frequency Domain Interferometry are given in International Patent Application No. PCT/US03/02349 and U.S. patent application No. 60/514,769, respectively. Polarization-sensitive OCT provides additional contrast by observing changes in the polarization state of reflected light. The first fiber-based implementation of polarization-sensitive time-domain OCT was described in Saxer et al., "High-speed fiber-based polarization-sensitive optical coherence tomography of in vivo human skin," *Opt. Lett.* 25, 1355 (2000).

In one exemplary technique of OCT, cross-sectional images of biological samples can be provided with a resolution on the scale of several to tens of microns. Contrast in the conventional OCT techniques can result from differences in the optical scattering properties of various tissues, and may permit imaging of tissue microstructures. Additional biological or functional information can be obtained by applying Doppler techniques to measure spatially-localized motion in the sample. These exemplary techniques, which can be referred to as Color Doppler OCT or Optical Doppler Tomography, have been used for imaging blood flow in skin, retina, esophagus, etc. Simultaneous imaging of tissue microstructure and blood flow can significantly enhance the diagnostic utility of OCT. Initial Doppler OCT measurements were performed with time-domain OCT (TD-OCT) systems, an example of which is shown in FIG. 1B.

Recently, it has been demonstrated that Fourier-Domain OCT (FD-OCT) provides significantly improved sensitivity, enabling high-speed imaging. FD-OCT has been implemented in two configurations, spectral-domain OCT ("SD-OCT") and optical frequency domain imaging ("OFDI"). In

SD-OCT, a spectrometer is used to record spectral fringes that result from the interference of a reference beam with light reflected from a sample. In OFDI, a narrowband wavelength-swept source and a single detector are used to record the same interferogram. Doppler imaging has been demonstrated recently in SD-OCT systems. An example of a Doppler SD-OCT system is shown in FIG. 1C. Doppler imaging using OFDI technique has not been demonstrated to our knowledge. OFDI procedure, however, may become the preferred imaging modality for several applications since it is less prone to motion artifacts associated with endoscopy and can provide a significantly larger depth range. Continued development of wavelength-swept laser sources promises further improvements in imaging speed and resolution. These advantages are compelling in several OCT applications, including Barrett's esophagus screening and coronary imaging. As such, flow imaging in many applications may require the development of phase-resolved OFDI.

Convention OCT systems and techniques create images based on the magnitude of the reflectivity as a function of depth. Additional information can be obtained by examining a phase of the reflectivity of the signal. Typically, a phase information of a signal can be meaningful when compared to another phase of the signal. This phase can be another measurement of the phase at a different depth or a measurement of phase at the same depth from a successive depth scan. Regardless of the exact implementation, the sensitivity of the image constructed from the phase measurements can be a function of the noise on the individual phase measurements and the repeatability of phase measurements.

In phase-resolved Doppler OFDI, it is possible for synchronization errors to induce spurious measurements of the interference fringe phases, resulting in a reduced performance. These synchronization errors can be referred to hereafter as timing-induced phase errors.

OBJECTS AND SUMMARY OF EXEMPLARY
EMBODIMENTS

To address and/or overcome the above-described problems and/or deficiencies, exemplary systems, methods and apparatus are provided for reducing the effect of the timing-induced phase errors. For example, in certain conventional methods, additional optical signals are generated and used to measure timing-induced errors so that they can be removed from the measured image. In other techniques, improved synchronization schemes can be presented to reduce the magnitude of the timing-induced phase noise directly.

According to the present invention, exemplary systems, methods and apparatus are provided for facilitating high-sensitivity depth-resolved phase measurements using an exemplary OFDI system. For example, a measurement of the phase can be used to measure blood flow and other motion in a turbid or scattering media, and can also be used to monitor optical thickness of materials over time or as a function of transverse location. Exemplary methods for achieving high-sensitivity in accordance with the exemplary embodiments of the present invention are also described herein. In one such exemplary method, a calibration signal can be generated and utilized to correct, modify and/or otherwise address timing-induced phase measurement errors. According to another exemplary embodiment of the present invention, the exemplary OFDI system may be modified to allow a simultaneous measurement of a calibration signal with the sample signal, and can also provide an exemplary procedure for correcting, modifying and/or otherwise addressing timing-induced phase measurements in the sample signal, e.g., by using such

calibration signal. In still another exemplary embodiment of the present invention, the calibration signal can be generated on a separate channel and acquired independently of the sample signal. For example, the calibration signal can be similarly used to correct errors in the sample signal. Additionally, according to a further exemplary embodiment of the present invention, method, apparatus and system can be provided for reducing, adjusting and/or minimizing timing-induced phase errors.

Thus, in accordance with one exemplary embodiment of the present invention, apparatus, system and method are provided which utilize signals received from a reference and a sample. In particular, a radiation is provided which includes at least one first electro-magnetic radiation directed to the sample and at least one second electro-magnetic radiation directed to the reference. A frequency of the radiation varies over time. An interference can be detected between at least one third radiation associated with the first radiation and at least one fourth radiation associated with the second radiation. It is possible to obtain a particular signal associated with at least one phase of at least one frequency component of the interference, and compare the particular signal to at least one particular information. Further, it is possible to receive at least one portion of the radiation and provide a further radiation, such that the particular signal can be calibrated based on the further signal.

For example, the particular information can include predetermined data. It is also possible to determine a further signal associated with at least one further phase of at least one further frequency component of the interference, and the at least one particular information can be the further signal. It is also possible to determine a further signal associated with at least one further phase of at least one further frequency component of a further interference, the further interference being different from the interference.

In another exemplary embodiment of the present invention, the further interference may be based on the radiation and the second radiation. The interference and the further interference may also be obtained at different times and/or at different locations of the sample. It is further possible to generate a further signal associated with the radiation, such that the particular information can be provided based on the further signal. In addition, it is possible to receive at least one portion of the radiation and provide a further radiation, and the particular signal and/or the particular information may be associated with the further radiation. In addition, it is possible to calibrate the particular signal based on the further signal. The calibration may be based on an actual distance and/or an optical distance between the sample and a particular arrangement. Further, it is possible to calibrate the particular signal based on an actual distance and/or an optical distance between the sample and the particular arrangement.

These and other objects, features and advantages of the present invention will become apparent upon reading the following detailed description of embodiments of the invention, when taken in conjunction with the appended claims.

BRIEF DESCRIPTION OF THE DRAWINGS

Further objects, features and advantages of the invention will become apparent from the following detailed description taken in conjunction with the accompanying figures showing illustrative embodiments of the invention, in which:

FIG. 1A is a schematic diagram of an exemplary embodiment of an OFDI system in accordance with the present invention;

FIG. 1B is a schematic diagram of a conventional Doppler TD-OCT system;

FIG. 1C is a schematic diagram of an exemplary embodiment of a spectral-domain OCT system in accordance with the present invention;

FIG. 2 is a schematic diagram of an exemplary embodiment of a portion of a system according to one exemplary embodiment of the present invention in which a sample arm that is modified to provide a calibration signal for measurement of timing-induced phase errors;

FIG. 3A is an exemplary graph illustrating a representative A-line resulting from the exemplary sample arm configuration depicted in FIG. 2;

FIG. 3B is an exemplary embodiment of a method for correcting the measured phase differences using this calibration mirror signal in accordance with the present invention;

FIG. 4 is an illustration of a distal end of a conventional OFDI probe showing the existing reflections of the distal end optics which can be used as the calibration signal;

FIG. 5 is an exemplary use of a phase-resolved OFDI probe to measure the blood flow in vivo in accordance with an exemplary embodiment of the present invention;

FIG. 6 is a schematic diagram of another exemplary embodiment of an OFDI system in accordance with the present invention in which the calibration signal is generated from an interferometer that is provided external to the OFDI interferometer;

FIG. 7 is a schematic diagram of yet another exemplary embodiment of the phase-resolved OFDI system in accordance with the present invention which can use an optical generation of the sample clock to synchronize the source wavelength-sweep and acquisition electronics;

FIG. 8 is a schematic diagram of still another exemplary embodiment of the phase-resolved OFDI system in accordance with the present invention that incorporates a frequency-shifter which can be driven with a signal derived from the DAQ sample clock;

FIG. 9 is an illustration of an exemplary use of the exemplary embodiment of the phase-resolved OFDI system to measure depth-resolved changes in optical path length as a function of time;

FIG. 10 is an illustration of an exemplary use of the exemplary embodiment of the phase-resolved OFDI system to measure depth-resolved changes in optical path length as a function of transverse displacement;

FIG. 11 is an exemplary graph of measured differential phases for the calibration mirror and a stationary mirror in the sample arm before and after correction for timing-induced phase errors according to an exemplary embodiment of the present invention;

FIG. 12 is an exemplary illustration of intensity and flow images of an Intralipid phantom as measured by the exemplary embodiment of the phase-resolved Doppler OFDI system according to the present invention;

FIGS. 13A-13C are exemplary illustrations of measurements of depth resolved flow in an Intralipid sample at high flow rates such that phase differences greater than π can be induced;

FIG. 14 is an exemplary illustration of measurements of blood flow in a human skin in vivo implemented using the exemplary embodiments of the present invention; and

FIG. 15 is a block diagram of an exemplary embodiment of a system in accordance with the present invention in which the calibration signal can be generated by a filter external to an interferometer and such signal can be combined with a balanced detection configuration.

5

Throughout the figures, the same reference numerals and characters, unless otherwise stated, are used to denote like features, elements, components or portions of the illustrated embodiments. Moreover, while the subject invention will now be described in detail with reference to the figures, it is done so in connection with the illustrative embodiments. It is intended that changes and modifications can be made to the described embodiments without departing from the true scope and spirit of the subject invention as defined by the appended claims.

DETAILED DESCRIPTION OF EXEMPLARY EMBODIMENTS

It should be understood that the exemplary embodiments of systems, software arrangements and methods in accordance with the present invention can be implemented in a variety of OCT systems and other systems in which signals from reference arm and sample arm can be interfered with one another to produce useful signals.

Exemplary Principle of Phase-Resolved Doppler FD-OCT

Exemplary Phase-resolved OCT techniques are described hereafter in the context of Fourier-Domain OCT, which is a category of OCT which is associated with the exemplary embodiments of the OFDI system according to the present invention. Fourier-Domain OCT can use an interference between two arms of an interferometer (e.g., a sample arm and a reference arm) to measure depth-dependent reflections in a turbid, semi-turbid and/or transparent medium. For example, an input light source is split into the reference arm and the sample arm. The light in the sample arm is directed to the sample to be imaged, and reflections from the sample are directed to a first port of an output coupler. The reference arm light is directed to the second port of the same output coupler. Spectral interference between the beams is measured by recording the interferometer output power as a function of wavelength. For a single reflection in the sample at position z where z denotes the total path-mismatch between the sample arm light and the reference arm light, the interferometer output can be provided as follows:

$$S(k=2\pi/\lambda) \sim P(k)\sqrt{R(z)}\cos(k2z+\phi_z) \quad (1)$$

where $S(k)$ is the output signal (optical power), $P(k)$ is the source power at k , $R(z)$ is the power reflectivity of the scatterer at position z , and ϕ_z is the phase of this reflection.

The reflectivity of the scatterer at position z is provided by the magnitude of the signal at frequency $2kz$. Typically, the detected signal is discretely sampled, meaning that the measured signal is recorded in n discrete samples of the continuous output $S(k)$. The discrete sampled output, S_l , is given by

$$S_l = P_l \sqrt{R(z)} \cos(k_l 2z + \phi_z), l=0 \dots (n-1) \quad (2)$$

where P_l is the source power at k_l . The discrete sampled output, S_l , is the discrete Fourier transformed (“DFT”) to yield the complex reflectivity profile, a_i , as a function of depth index i ,

$$a_i = DFT(S_l). \quad (3)$$

The signal from the scatterer at position z is contained in the complex reflectivity profile coefficient a_m , where m is the depth index corresponding to position z . For example, each measurement of the discrete sampled output, S_l , can yield a single measurement of the complex reflectivity profile as a function of depth (A-line). The motion of the scatterer at depth index i results in a change in the phase, Φ_i , of the complex reflectivity profile coefficient a_i ($\Phi_i = \text{angle}(a_i)$). If the complex reflectivity profile is provided with depth index i

6

for A-line j as $a_{i,j}$, then a displacement of δ_z between A-lines j and $j-1$ can yield a phase change given by:

$$\Delta\Phi_{i,j} = (\Phi_{i,j} - \Phi_{i,j-1}) = 2n < k > \delta_z. \quad (4)$$

The phase-resolved FD-OCT can measure motion in the scattering medium by calculating these phase differences at the sample depth for successive A-lines.

Phase-Resolved Doppler OFDI Technique

FD-OCT techniques of SD-OCT and OFDI systems and methods can both measure the discrete spectral interference S_l . However, these techniques generally differ in the implementation of this measurement. The OFDI systems and methods can use a wavelength-swept source and a single-element photoreceiver (and/or a set of single-element photoreceivers) to record S_l as a function of time. FIG. 1A shows a block diagram of an exemplary embodiment of a high-speed OFDI technique for imaging at least a portion of a sample. The exemplary system shown in FIG. 1A includes three modules **85**, **90** and **95**, e.g., a wavelength-swept source **85**, an interferometer **90**, and acquisition electronics arrangement **95**. The wavelength-swept source **85** (hereafter referred to as a swept source) can be provided as a ring-cavity laser. The swept source **85** can include a semiconductor optical amplifier (“SOA”) **125** as a gain element and a polygon mirror filter **101**. The polygon mirror filter **101** can include a polygon mirror **100**, telescope **105**, diffraction grating **110**, and fiber collimator **113**. A polarization controller **120** may be included to optimize the laser polarization, and an output coupler **130** may provide a laser output. The output coupler nominally splits light equally between the output port **132** and laser port **131**. An optical circulator **115** directs light from the laser port **131** to the polygon mirror filter **101**, and directs light returning from the polygon mirror filter **101** to the polarization controller **120**. As the polygon mirror **100** rotates, the wavelength reflected from the polygon mirror filter **101** sweeps in wavelength, causing the laser output to sweep in wavelength in a similar manner.

The laser output at a port **132** can therefore be wavelength swept in time. This output is input to an interferometer which includes an interferometer coupler **135** which splits the light into a reference arm port **135a** and sample arm port **135b**. The reference arm light is split by a coupler **165**. The light from an output port **165a** of the coupler **165** is directed to a second circulator **145** which passes the light to a fiber Bragg grating (“FBG”) **150**. The FBG **150** has a narrowband reflection at a discrete wavelength within the wavelength-sweep range of the source. As the source **85** tunes past this reflection wavelength, a reflected optical pulse is generated. This pulse can be directed by a circulator **145** to a photoreceiver **155**, and such directed pulse is converted into a TTL pulse by a TTL pulse generator **160**. This TTL pulse can be used as a trigger signal for data acquisition electronics **200**. The light from another output port **165b** of the coupler is directed to a third circulator **170** which directs the light to a variable optical delay **210**. This variable optical delay is used to path-match the interferometer **90**. The return light is directed by the circulator **170** to a polarization controller **175**, followed by a polarizer **180**, and finally to a first port **185a** of an output coupler **185**. The sample arm light at the sample arm port **135b** is directed to a fourth circulator **205**, which in turn directs the light on fiber **206** to the sample to be imaged. Imaging optics **215** can focus the light on the sample, and allow for a beam translation. The light reflected from the sample is collected by the same fiber **206**, and returned to the fourth circulator **205** which directs the light to a second port **185b** of the output coupler **185**.

The reference arm light and the sample arm light interfere at the output coupler **185**. This interference signal is detected

by a photoreceiver **190a** on an output port **185c** and a photoreceiver **190b** on another output port **185d**. The signals from these photoreceivers **190a**, **190b** are subtracted in a unit **195**, and directed toward an analog-to-digital (A-D) input port of a data acquisition (DAQ) board **200**.

The DAQ board **200** can acquire n samples at a clock rate f_{cl} , where n is predetermined. The clock signal can be internally generated in the DAQ board **200**. The trigger signal from the TTL pulse generator **160** may originate from the optical pulse produced by the FBG **150**. A lack of synchronization between the trigger pulse and the internal DAQ sample clock may cause a variable delay between the arrival of the trigger pulse and the first analog-to-digital conversion. This delay can be effected by one full sample clock period. Thus, if the sweep of the source is identified by $k_l = k_o + a_k l$, the sampled fringe for A-line j , $S_{i,j}$, can be given by

$$S_{i,j} \sim P_j \sqrt{R(z)} \cos((k_o + a_k(l + \Delta_j))2z + \phi_z), l=0 \dots (n-1) \quad (5)$$

where Δ_j can vary between 0 and 1 depending on the relative timing of the sample clock and the trigger pulse. The measured phase difference between successive A-lines for a stationary scatterer at position z can be given by:

$$\Delta\Phi_{i,j} = a_k 2z (\Delta_j \Delta_{j-1}) \quad (6)$$

The phase difference results from timing variations in the acquisition time (described by Δ_j) and masks phase differences resulting from sample motion, degrading the system sensitivity. Writing the Nyquist limited making imaging depth as $z_{Ny} = \lambda / (2a_k)$ and using the normalized depth factor $\Gamma_z = z / z_{Ny}$, the timing-induced phase errors can be described by:

$$\Delta\Phi_{i,j} < \Gamma_z \pi. \quad (7)$$

The above-described procedure in accordance with the present invention indicates that timing-induced phase errors increase linearly with depth up to, e.g., a maximum value of π at $\Gamma_z = 1$.

Correction of Timing-Induced Phase Errors through a Generation of a Calibration Signal

According to one exemplary embodiment of the present invention, an additional signal can be generated by the exemplary system described herein and utilized to measure and subsequently correct for the timing-induced phase errors. For example, FIG. 2 shows an exemplary embodiment of such exemplary system in accordance with the present invention in which the sample arm is modified to facilitate the generation of the additional calibration signal. FIG. 2 shows that exemplary details of the sample arm which is after the optical circulator **205** illustrated in FIG. 1. As shown in FIG. 2, the light on a fiber **300** (i.e., the fiber **206** of FIG. 1A) can be split by a coupler **305**. The light on a port **305a** can be directed to a calibration mirror **310** that may have a variable optical delay. The light on a port **305b** can be directed to the sample **320** in a similar manner to that of FIG. 1A. The interferometer output signal forwarded from the calibration mirror can be localized in depth, and the variable optical delay may be adjusted such that it is located near the maximum imaging depth (and thus does not significantly obscure the image resulting from the sample optics **320**). The magnitude of the signal resulting from the variable optical delay can be adjusted such that it is significantly greater than that originating from the sample at that depth but not large enough such that significant auto-correlation noise is induced.

FIG. 3A shows a graph **350** of an exemplary A-line resulting from the exemplary system configuration illustrated in FIG. 2. A signal **360** from the calibration mirror is clearly seen among a sample (tissue) reflectance signal **355**. A flow dia-

gram of an exemplary embodiment of a method for correcting the measured phase differences using this calibration mirror signal in accordance with the present invention is shown in FIG. 3B, and provided as follows:

- 5 (1) Determine/calculate the DFT of each measured A-line, $a_{i,j} = \text{DFT}(S_{i,j})$ —step **370**.
- (2) Determine/calculate an angle $\Phi_{i,j} = \text{unwrap}(\text{angle}(a_{i,j}))$ where unwrap is a standard phase unwrapping algorithm which operates along the dimension j —step **375**.
- 10 (3) Determine/calculate a phase difference between adjacent A-lines $\Delta\Phi_{i,j} = \Phi_{i,j} - \Phi_{i,j-1}$ —step **380**, and
- (4) Determine/calculate a corrected phase difference, $\Delta\Phi'_{i,j}$, as $\Delta\Phi'_{i,j} = \Delta\Phi_{i,j} - (i/k)\Delta\Phi_{k,j}$, where k is a depth index of the calibration mirror signal—step **385**.

15 In a further embodiment, existing reflections from the optical probe are used as the calibration signal. FIG. 4 shows an exemplary embodiment of a distal-end optics portion of an exemplary OCT probe in accordance with the present invention. As shown in FIG. 4, light may be transmitted on a fiber **400** to a collimating lens **410**, a right-angle prism **420**, and finally the light **430** exits the prism to the sample **440** to be imaged **440**. Discrete reflections can occur at any of the interfaces between the components, and the signal from these reflections can be utilized as a calibration signal in addition to and/or instead of the calibration mirror **310** of FIG. 2.

25 In a further exemplary embodiment of the system according to the present invention shown in FIG. 6, the calibration signal can be generated by an optical setup that may be external to an OFDI interferometer, and detected on a second detector that is sampled synchronously with the detector that samples the OFDI system output. In particular, a source **550** output can be split by a coupler **560** which directs a first portion of light to an OFDI interferometric system **561** and a second portion of light to a calibration signal generator **562**. The OFDI interferometric system **561** includes couplers **565** which provide signals to the reference arm and the sample arm, and the signal in the reference arm is forwarded to a coupler **575** which then forwarded a signal therefrom to a receiver **580**. In the sample arm, the signal is forwarded to another coupler **570**, which also receive the signal from the coupler **575**, and then provide a signal to a portion **585** of the sample **590**. The calibration signal generator **562** includes a periodic optical filter **595** which facilitates a generation of an intensity modulated optical signal, that is then detected at a receiver **596**. The periodic optical filter **595** can be, for example, a Fabry-perot etalon, a Mach-Zehnder interferometer, or a Michelson interferometer. The calibration signal and the OFDI signal may be detected on DAQ Channel 1 (shown as element **597**) and a DAQ channel 2 device (shown as element **598**), respectively. These channels can be sampled synchronously. Changes in acquisition timing may affect the phase of this calibration signal similarly to that described above when the calibration signal was generated with a mirror in the sample arm. Thus, the calibration signal detected on the DAQ channel 1 can be used to correct for timing-induced phase errors. Alternately or in addition, the calibration signal and the OFDI signal can be combined electronically, e.g., after the detection and before the analog-to-digital conversion, thus enabling both to be sampled by the same analog-to-digital channel.

60 In a further exemplary embodiment of the system according to the present invention which is shown in FIG. 15, a balanced detection can be effectuated by balancing a signal channel that carries interference between the sample arm and the reference arm with a non-signal carrying reference path. As previously discussed, a source **900** can provide the electromagnetic radiation (e.g., a laser beam) to a polarization con-

troller **905** may be included to optimize the laser polarization, and a fiber splitter **915** can receive the signal from the controller **905**. The fiber splitter **915** splits light to be forwarded to different paths. In one path, for example, a reference interference to calibrate the Doppler measurements can be generated in the non-signal carrying reference, e.g., by introducing a Fabry-Perot cavity **955** in the non-signal carrying reference (as indicated in the dashed box in FIG. **15**) which receives the radiation from the splitter **915**. The modulation depth on the reference as a function of wavelength as introduced by the Fabry-Perot cavity **955** should be small enough as to not affect the balanced detection scheme, and strong enough to provide a good calibration signal. Then, the cavity **955** forwards the resultant radiation to a variable attenuator, and then detected by balanced detectors D_1 and D_2 (**945**, **950**). In the other path, a polarization modulator or birefringent material **915** receives the split respective signal, and forwards it to a circulator **920** that directs one portion of the radiation to another fiber splitter **925** and splits the received signal to be forwarded to a sample arm and to a reference arm (and possibly to an optional polarizer **930**), and directs light returning therefrom to a polarization controller **935**, which then provides the polarized radiation to a polarization splitter **940** that also forwards the polarized split radiation to detectors D_1 and D_2 (**945**, **950**).

Correction of Timing-Induced Phase Errors through Post-Processing

In still another exemplary embodiment of the system, arrangement and method according to the present invention, phase measurements can be corrected without the use of a calibration mirror. In this exemplary technique, a intensity-weighted linear fit can be applied to each measured phase difference line, $\Delta\Phi_{i,j}$, as a function of depth index i , $y_{i,j}=m_j i + b_j$. The corrected phase differences can be given by $\Delta\phi_{i,j}= \Delta\Phi_{i,j} - m_j i - b_j$.

Correction of Timing-Induced Phase Errors through the Improved Acquisition/Source Synchronization

In a further embodiment, the timing-induced phase errors are reduced by improving the synchronization between the swept source and the DAQ board. The rotational speed of the polygon mirror **100** of FIG. **1A** can be determined by the frequency of a signal input to the polygon mirror driver (not shown). If such signal is generated from the same clock as the one which generates the sample clock of the DAQ board, and the polygon mirror driver can maintain adequate phase-locking between the polygon and drive signal, then the synchronization between the wavelength-sweep and the data acquisition can be achieved. In this case, the delay of Eq. 5 denoted by Δ_j can remain constant, and thus the timing-induced phase errors may be reduced.

In a still further exemplary embodiment of the system according to the present invention that is shown in FIG. **7**, an acquisition sample clock can be generated optically by using a periodic filter such as a Fabry-Perot etalon, a Mach-Zehnder interferometer, and/or a Michelson interferometer. As shown in FIG. **7**, a portion of a swept source **600** can be directed to a sample clock generator **606** which can include a periodic optical filter **610**, a receiver **615** and a TTL generating circuit **620**. The periodic optical filter **610** can produce an oscillating output signal which is detected at the receiver **615**. The receiver output is directed to the TTL generating circuit **620** which can include voltage comparators and/or Schmitt triggers to generate a TTL pulse train. This pulse train can be input into a DAQ external sample clock input port **655** to be used as a sample clock. Because sampling can be synchronized to the laser wavelength sweep through the sample clock generator, the timing-induced noise can be reduced directly.

This technique can be used separately or in combination with previously described techniques for correcting phase errors. Applications of Phase-Resolved OFDI

In still another exemplary embodiment of the present invention, the phase-resolved OFDI system can be used to image blood flow distributions during an intravascular OFDI imaging. An exemplary device capable of imaging blood flow is shown in FIG. **5**. For example, an exemplary optical probe **510** in accordance with the present invention can be placed inside an artery **520**, and the imaging beam **500** can be emitted from a side of the probe **510**. The depth resolved blood flow can be detected, and if the probe is rotated, a 2D map of the blood flow may be created. The end view illustrates the rotation of the imaging beam. Alternately, a forward looking probe can be provided for imaging the blood ahead of the probe **510**.

In yet another exemplary embodiment of a phase-resolved OFDI system of the present invention which is shown in FIG. **8**, a frequency shifter can be provided therein. For example, a frequency shifter **711** can be used to enable a doubling of the imaging depth. If the frequency shifter **711** is driven with a signal that is unsynchronized with the sampling clock, noise in the measured phase may result. In the exemplary embodiment of the system shown in FIG. **8**, the frequency shifter is driven with a signal derived from the sample clock. Light is output from the source and split into a reference arm and a sample arm by the first splitter **710**. The reference arm contains a frequency shifter **712** and the sample arm contains the same frequency shifter **711**. Generally, only one of the frequency shifters **711**, **712** can be actively driven, and the other one of the shifters **711**, **712** may be used to compensate for the dispersion of the driven frequency shifter. The frequency shifter that is not driven can alternatively be a dispersion compensating element. The frequency shifter **712** in the reference arm may be driven through a signal carried on line **713** which can be derived from a DAQ sample clock output **725**. This output clock **725** may be down-shifted in frequency using a "Divide by N" digital logic circuit **720**, and the resulting signal can pass through an amplifier and filter stage **715** to produce a single tone on line **713**. Because the drive signal for the frequency shifter may be driven by the DAQ sample clock output **725**, the phase of the frequency shift may be synchronous with the sample clock, and thus does not necessarily induce additional phase noise. Various exemplary techniques in accordance with the present invention described herein can be used to correct for any residual timing-induced noise.

In a further exemplary embodiment of the phase-resolved OFDI system of the present invention, such system can be used to determine variations in the optical-path length between two points in depth as a function of time. For example, FIG. **9** illustrates an illustration of an exemplary use of the exemplary embodiment of the phase-resolved OFDI system to measure depth-resolved changes in optical path length as a function of time. This use is provided for the case of a object between a first reflective surface **805** at depth $z1$ and a second reflective surface **810** at depth $z2$. Between the reflective surfaces **805**, **810** is an object to be imaged **815**. The reflective surfaces **805**, **810** can either be fixed external surfaces such as glass slides or structural features of the biological object itself. By monitoring the phase of the signals due to the reflections off these surfaces **805**, **810**, the optical path length between $z1$ and $z2$ can be monitored, allowing changes in the object to be monitored. These potential changes can include variations in the object index of refraction with time, or expansion of the object in time. In the illustration of FIG. **9**, the imaging beam can be held stationary, and used to monitor changes at a fixed transverse point over time.

A further exemplary illustration of an exemplary use of the exemplary embodiment of the phase-resolved OFDI system to measure depth-resolved changes in an optical path length as a function of transverse displacement. An imaging beam **850** is directed toward a sample object located between a first reflective surface **855** and a second reflective surface **865**. The optical path length difference between these reflective surfaces **855**, **865** is known by the design of the system and/or a prior measurement before an object **860** is inserted. The phase of the reflective surfaces **855**, **865** can be measured as a function of a transverse displacement of the imaging beam **850**, and the variations in the transverse optical path length of the object **860** can be found by comparing the phase difference between the two signals with the phase difference as measured and/or known previously without the object being present. For example, if the system is has enough stability, the first surface reflectance at z_1 may not be needed.

It can be appreciated by those skilled in the art that one of the embodiments can be used in combination with other exemplary embodiments described herein to provide various phase-resolved OFDI systems with reduced timing-induced phase noise in accordance with the present invention.

EXAMPLE

The exemplary embodiment(s) of the system, apparatus and method according to the present invention have been verified as follows:

The phase differences between successive A-lines were measured in the exemplary configuration of FIG. 2 with a stationary sample mirror in the sample arm. FIG. 11 an exemplary graph **1010** of measured differential phases for the calibration mirror and a stationary mirror in the sample arm before and after a correction for timing-induced phase errors according to an exemplary embodiment of the present invention. The calibration mirror signal **1015** and the uncorrected sample signal **1020** show phase errors of the magnitude predicted by Eq. 7. The corrected phase measurements **1025** show substantial reduction in spurious phase differences.

FIG. 12 shows an illustration of measurements taken of Intralipid (scattering liquid) flow through a tube immersed in the same stationary Intralipid. Both the OFDI intensity image **1030** and the flow image **1035** are shown. The presence of flow is clearly detected by the phase-resolved OFDI system of an exemplary embodiment of the present invention.

FIGS. 13A-13C show illustrations of a measurement of Intralipid flow through a tube in which the flow rate is large enough that phase differences greater than π are induced. In the graph of FIG. 13A, the depth resolved flow **1040** as a function of time is plotted. In the graph of FIG. 13B, the measured phase differences **1045** are unwrapped to remove discontinuities of 2π such that the large flow profile can be measured. FIG. 13C shows the graph of the unwrapped flow profile **1050** at time T as marked in FIGS. 13(a) and 13(b). This shows the ability of phase-resolved OFDI to measure large flow rates that induced phase differences greater than π without the deleterious effects of fringe washout.

FIG. 14 shows an illustration of a phase-resolved measurement of blood flow in vivo near the nail bed of a human finger. Vessels are clearly shown in the flow image **1055** that do not appear in the intensity image **1060**.

The foregoing merely illustrates the principles of the invention. Various modifications and alterations to the described embodiments will be apparent to those skilled in the art in view of the teachings herein. Indeed, the arrangements, systems and methods according to the exemplary embodiments of the present invention can be used with and/or

implement any OCT system, OFDI system, SD-OCT system or other imaging systems, and for example with those described in International Patent Application PCT/US2004/029148, filed Sep. 8, 2004 which published as International Patent Publication No. WO 2005/047813 on May 26, 2005, U.S. patent application Ser. No. 11/266,779, filed Nov. 2, 2005 which published as U.S. Patent Publication No. 2006/0093276 on May 4, 2006, and U.S. patent application Ser. No. 10/501,276, filed Jul. 9, 2004 which published as U.S. Patent Publication No. 20050018201 on Jan. 27, 2005, the disclosures of which are incorporated by reference herein in their entirety. It will thus be appreciated that those skilled in the art will be able to devise numerous systems, arrangements and methods which, although not explicitly shown or described herein, embody the principles of the invention and are thus within the spirit and scope of the present invention. In addition, to the extent that the prior art knowledge has not been explicitly incorporated by reference herein above, it is explicitly being incorporated herein in its entirety. All publications referenced herein above are incorporated herein by reference in their entirety.

What is claimed is:

1. An apparatus comprising:

at least one hardware first arrangement including a source which provides a radiation which includes at least one first electro-magnetic radiation directed to a sample and at least one second electro-magnetic radiation directed to a reference, wherein a frequency of the radiation provided by the at least one first arrangement varies over time; and

at least one hardware second arrangement which includes a detector that detects a particular interference signal between at least one third radiation associated with the at least one first radiation and at least one fourth radiation associated with the at least one second radiation,

wherein that particular interference signal is detected by the detector across a first radiation frequency range,

wherein the at least one second arrangement obtains at least one first phase of at least one frequency component of the particular interference signal, and wherein the at least one second arrangement includes a hardware computing arrangement which compares the at least one first phase with at least one second phase of at least one frequency component of a previously-detected interference signal which is detected by the detector across a second radiation frequency range, and

wherein the hardware computing arrangement generates at least one image of at least one portion of the sample that substantially excludes information caused by a difference between the first and second radiation frequency ranges based on the comparison and as function of the interference signals.

2. The apparatus according to claim 1, wherein the at least one second arrangement is configured to determine a signal associated with at least one further phase of at least one further frequency component of a further interference signal, and wherein the at least one second phase is associated with the signal.

3. The apparatus according to claim 1,

wherein the at least one second arrangement is configured to determine a signal associated with at least one further phase of a further interference signal, the further interference signal being different from the particular and previously-detected interferences.

4. The apparatus according to claim 3, wherein the at least one second arrangement obtains the particular and previously-detected interference signals at different times.

13

5. The apparatus according to claim 3, wherein the at least one second arrangement obtains the particular and previously-detected interference signals at different locations of the sample.

6. The apparatus according to claim 1, comprising a further reference configure to receive at least one portion of the radiation and provide a further radiation so as to generate a signal, wherein at least one of the signal or the at least second phase is associated with the further radiation.

7. The apparatus according to claim 6, wherein the at least one second arrangement is configured to calibrate the at least one first phase based on the signal.

8. The apparatus according to claim 7, wherein the calibration is based on at least one of an actual distance or an optical distance between the sample and the first arrangement.

9. The apparatus according to claim 1, wherein the at least one second arrangement is configured to calibrate the signal based on at least one of an actual distance or an optical distance between the sample and the first arrangement.

10. The apparatus according to claim 1, further comprising:

at least one hardware third arrangement including a further reference which receives at least one portion of the radiation and provides a further radiation which is at least partially based on the radiation, wherein the hardware computing arrangement induces a phase shift of the particular phase based on the further radiation, and wherein the further radiation is independent of any property of the sample.

11. The apparatus according to claim 10, wherein the at least one hardware third arrangement is provided in the sample arm.

12. The method according to claim 10, wherein the reference includes a mirror that is positioned to directly reflect the at least one portion to the at least one second arrangement.

13. The apparatus according to claim 10, wherein the further radiation is distinct from the at least one second radiation and the at least one fourth radiation.

14. The apparatus according to claim 10, wherein the at least one first arrangement includes a single laser source which generates the radiation.

15. The apparatus according to claim 10, wherein the computing arrangement induces the phase shift at least one of digitally or mathematically.

16. The apparatus according to claim 1, wherein the at least one second arrangement detects a further signal corresponding to a further interference signal between the at least one second and third radiations, and wherein the further signal is associated with at least one phase of at least one frequency component of an additional interference associated with the further signal.

17. The apparatus according to claim 1, wherein the at least one second arrangement determines image information based on the comparison between the first and second phases.

18. A method comprising:

providing a radiation which includes at least one first electro-magnetic radiation directed to a sample and at least one second electro-magnetic radiation directed to a reference, wherein a frequency of the radiation varies over time;

detecting a particular interference signal between at least one third radiation associated with the at least one first radiation and at least one fourth radiation associated with the at least one second radiation, wherein the particular interference signal is detected across a first radiation frequency range;

14

obtaining at least one first phase of at least one frequency component of the particular interference signal; and with a hardware computer arrangement, comparing the at least one first phase with at least one second phase of at least one frequency component of a previously-detected interference signal which is detected by across a second radiation frequency range, and

with the hardware computer arrangement, generating at least one image of at least one portion of the sample that substantially excludes information caused by a difference between the first and second radiation frequency ranges based on the comparison and as function of the interference signals.

19. The method according to claim 18, further comprising determining a signal associated with at least one further phase of a further interference signal, the further interference signal being different from the particular and previously-detected interference signals.

20. The method according to claim 18, further comprising: determining a signal associated with at least one further phase of a further interference signal, the further interference signal being different from the particular and previously-detected interference signals.

21. The method according to claim 20, further comprising obtaining the particular and previously-detected interference signals at different times.

22. The method according to claim 20, further comprising obtaining the particular and previously-detected interference signals at different locations of the sample.

23. The method according to claim 18, further comprising: receiving at least one portion of the radiation and provide a further radiation so as to generate a signal, wherein at least one of the signal or the at least second phase is associated with the further radiation.

24. The method according to claim 23, further comprising: calibrating the at least one first phase based on the signal.

25. The method according to claim 24, wherein the calibration is based on at least one of an actual distance or an optical distance between the sample and a particular arrangement.

26. The method according to claim 18, further comprising: calibrating the second signal based on at least one of an actual distance or an optical distance between the sample and a particular arrangement.

27. The method according to claim 18, further comprising: receiving at least one portion of the radiation and provide a further radiation which is at least partially based on the radiation; and

inducing a phase shift of the particular phase based on the further radiation, and wherein the further radiation is independent of any property of the sample.

28. The method according to claim 27, wherein the at least one portion of the radiation is received in the sample arm.

29. The method according to claim 27, wherein the further radiation is distinct from the at least one second radiation and the at least one fourth radiation.

30. The method according to claim 27, wherein the radiation is generated by a single laser source.

31. The method according to claim 27, wherein the phase shift is induced at least one of digitally or mathematically.

32. The method according to claim 18, further comprising detecting a further signal corresponding to a further interference signal between the at least one second and third radiations, and wherein the signal is associated with at least one phase of at least one frequency component of an additional interference signal associated with the further signal.

15

33. The method according to claim **18**, further comprising imaging information based on the comparison between the first and second phases.

34. A system comprising:

at least one hardware first arrangement including a detector 5
 which detects an interference signal between at least one
 first radiation associated with a first split portion of a
 radiation received from a sample and a second split
 portion of the radiation received from a reference,
 wherein a frequency of the radiation varies over time, 10
 wherein the interference signal is detected by the detec-
 tor across a first radiation frequency range, wherein the
 at least one arrangement obtains at least one first phase
 of at least one frequency component of the interference
 signal, wherein the at least one detector arrangement 15
 includes a one hardware computing second arrangement
 which compares the at least one first phase with at least
 one second phase of at least one frequency component of

16

a previously-detected interference signal which is
 detected by the detector across a second radiation fre-
 quency range, and wherein the one hardware computing
 second arrangement generates at least one image of at
 least one portion of the sample that substantially
 excludes information caused by a difference between
 the first and second radiation frequency ranges based on
 the comparison and as function of the interference sig-
 nals.

35. The apparatus according to claim **34**, wherein the at
 least one hardware first arrangement detects a further signal
 corresponding to a further interference signal between the
 first and second split portions of the radiation, and wherein
 the previously-detected interference signal is associated with
 at least one phase of at least one frequency component of an
 interference signal associated with the further signal.

* * * * *