

(12) **United States Patent**
Bourang

(10) **Patent No.:** **US 9,254,210 B2**
(45) **Date of Patent:** **Feb. 9, 2016**

(54) **MULTI-STENT AND MULTI-BALLOON APPARATUS FOR TREATING BIFURCATIONS AND METHODS OF USE**

USPC 623/1.35, 1.11, 1.16
See application file for complete search history.

(71) Applicant: **Advanced Bifurcation Systems, Inc.**,
Los Angeles, CA (US)

(56) **References Cited**

(72) Inventor: **Henry Bourang**, Turlock, CA (US)

U.S. PATENT DOCUMENTS

(73) Assignee: **Advanced Bifurcation Systems, Inc.**,
Los Angeles, CA (US)

4,069,825 A 1/1978 Akiyama
4,468,224 A 8/1984 Enzmann et al.

(Continued)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 302 days.

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **13/796,466**

CN 1441654 A 10/2003
CN 1867374 A 11/2006

(22) Filed: **Mar. 12, 2013**

(Continued)

(65) **Prior Publication Data**

US 2013/0268047 A1 Oct. 10, 2013

OTHER PUBLICATIONS

Office Action of Japanese Patent Application No. 2011-529290, mailed Sep. 25, 2013, 5 pages.

(Continued)

Related U.S. Application Data

(63) Continuation of application No. PCT/US2012/024366, filed on Feb. 8, 2012.

Primary Examiner — Katrina Stransky

Assistant Examiner — Katherine Schwiker

(60) Provisional application No. 61/440,742, filed on Feb. 8, 2011.

(74) *Attorney, Agent, or Firm* — Kilpatrick Townsend and Stockton LLP

(51) **Int. Cl.**

A61F 2/954 (2013.01)

A61F 2/95 (2013.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61F 2/954** (2013.01); **A61F 2/958** (2013.01); **A61F 2/852** (2013.01);

(Continued)

(58) **Field of Classification Search**


CPC A61F 2/06; A61F 2/852; A61F 2/954; A61F 2/958; A61F 2/856; A61F 2002/826; A61F 2002/065; A61F 2002/067; A61F 2002/61; A61F 2/95; A61F 2002/061; A61M 2025/0004; A61M 2025/045; A61M 25/104

(57)

ABSTRACT

A system for treating a bifurcated vessel that includes a first delivery catheter and a second delivery catheter. The first delivery catheter carries a proximal first stent and a distal second stent. The first delivery catheter also has a first elongate shaft, a proximal first expandable member with the proximal first stent disposed thereover, and a distal second expandable member with the distal second stent disposed thereover. The proximal first expandable member and distal second expandable member are independently expandable of one another. The second delivery catheter carries a third stent. The second delivery catheter also has a second elongate shaft, and a third expandable member with the third stent disposed thereover. The third expandable member is independently expandable of the proximal first expandable member and the distal second expandable member.

19 Claims, 18 Drawing Sheets

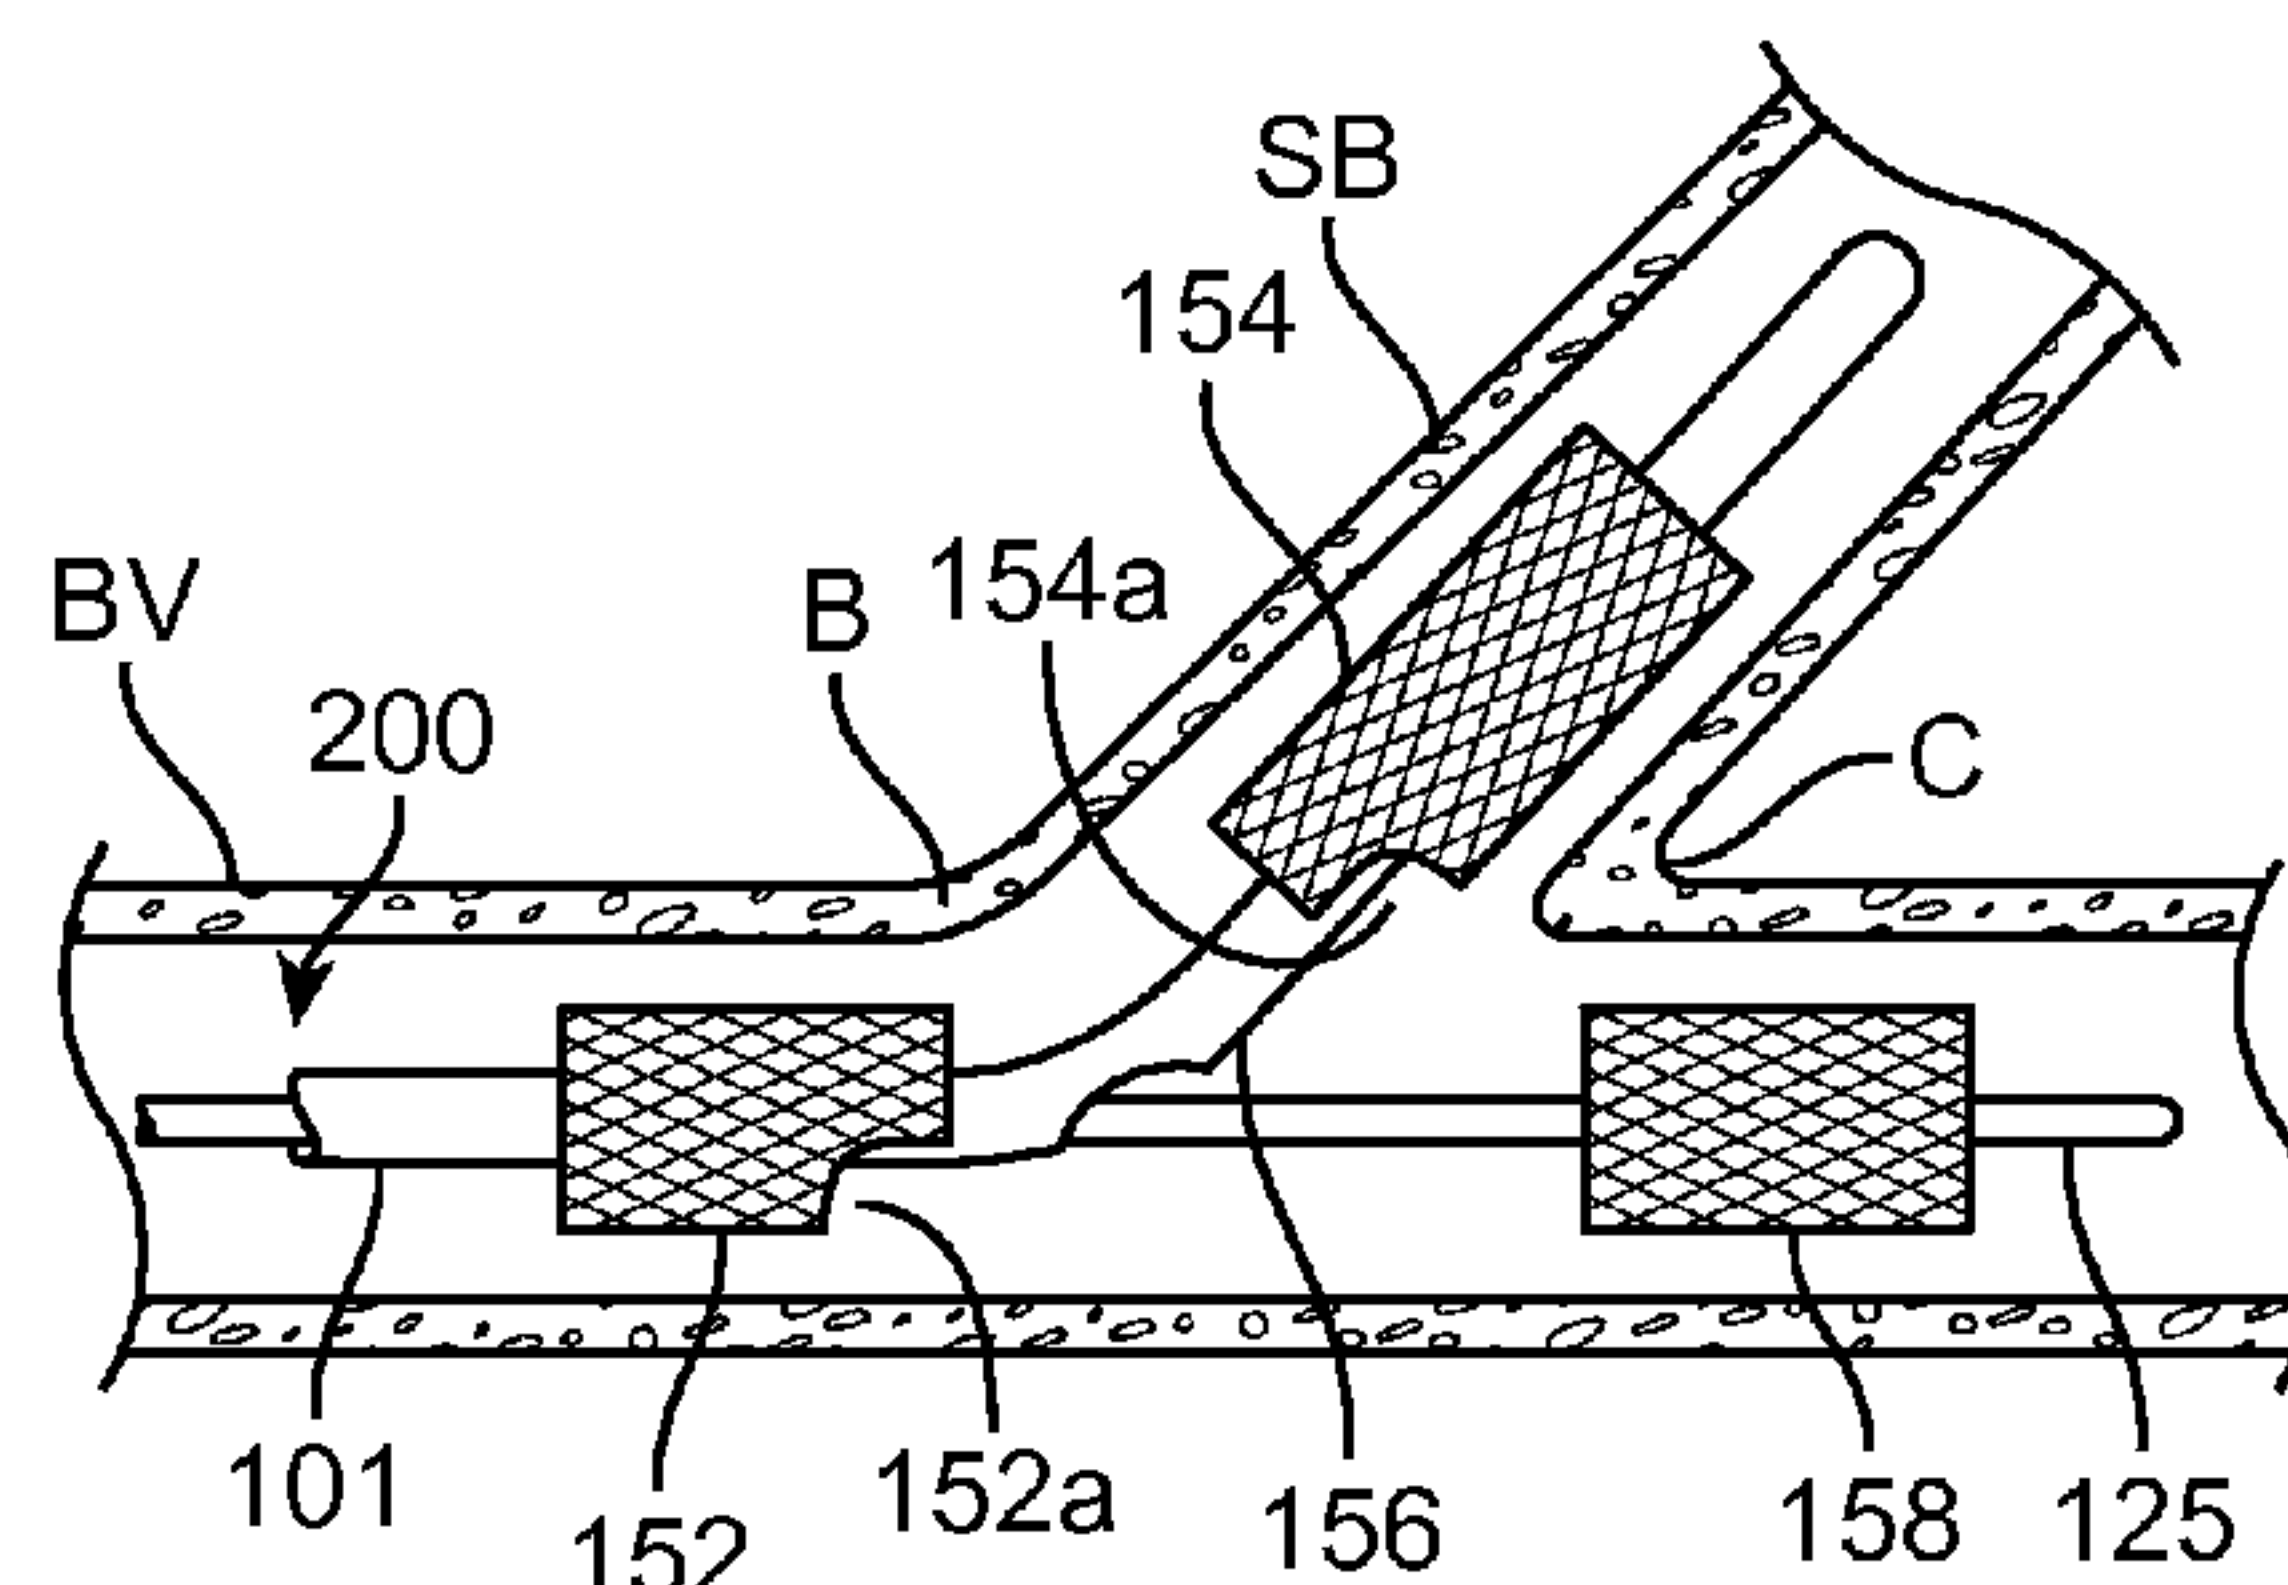

(51)	Int. Cl.		5,632,763 A	5/1997	Glastra
	<i>A61F 2/06</i>	(2013.01)	5,632,772 A	5/1997	Alcime et al.
	<i>A61F 2/958</i>	(2013.01)	5,634,928 A	6/1997	Fischell et al.
	<i>A61F 2/852</i>	(2013.01)	5,639,274 A	6/1997	Fischell et al.
	<i>A61F 2/82</i>	(2013.01)	5,662,675 A	9/1997	Polanskyj Stockert et al.
	<i>A61M 25/10</i>	(2013.01)	5,669,924 A	9/1997	Shaknovich
	<i>A61M 25/00</i>	(2006.01)	5,670,161 A	9/1997	Healy et al.
(52)	U.S. Cl.		5,676,654 A	10/1997	Ellis et al.
	CPC	<i>A61F 2002/061</i> (2013.01); <i>A61F 2002/826</i>	5,683,451 A	11/1997	Lenker et al.
		(2013.01); <i>A61M 25/104</i> (2013.01); <i>A61M</i>	5,697,948 A	12/1997	Marin et al.
		<i>2025/0004</i> (2013.01); <i>A61M 2025/1045</i>	5,697,967 A	12/1997	Dinh et al.
		(2013.01)	5,702,418 A	12/1997	Ravenscroft
			5,709,701 A	1/1998	Parodi
			5,716,393 A	2/1998	Lindenberg et al.
			5,722,669 A	3/1998	Shimizu et al.
			5,723,003 A	3/1998	Winston et al.
			5,735,869 A	4/1998	Fernandez-Aceytuno
			5,741,323 A	4/1998	Pathak et al.
			5,749,848 A	5/1998	Jang et al.
			5,749,921 A	5/1998	Lenker et al.
(56)	References Cited		5,755,735 A	5/1998	Richter et al.
	U.S. PATENT DOCUMENTS		5,755,771 A	5/1998	Penn et al.
	4,512,338 A	4/1985 Balko	5,755,772 A	5/1998	Evans et al.
	4,564,014 A	1/1986 Fogarty et al.	5,755,776 A	5/1998	Al-Saadon
	4,580,568 A	4/1986 Gianturco	5,755,781 A	5/1998	Jayaraman
	4,681,110 A	7/1987 Wiktor	5,769,882 A	6/1998	Fogarty et al.
	4,690,684 A	9/1987 McGreevy et al.	5,772,669 A	6/1998	Vrba
	4,733,665 A	3/1988 Palmaz	5,776,141 A	7/1998	Klein et al.
	4,739,762 A	4/1988 Palmaz	5,797,951 A	8/1998	Mueller et al.
	4,762,129 A	8/1988 Bonzel	5,800,519 A	9/1998	Sandock
	4,770,176 A	9/1988 McGreevy et al.	5,807,398 A	9/1998	Shaknovich
	4,775,337 A	10/1988 Van Wagener et al.	5,824,040 A	10/1998	Cox et al.
	4,776,337 A	10/1988 Palmaz	5,824,041 A	10/1998	Lenker et al.
	4,886,062 A	12/1989 Wiktor	5,827,320 A	10/1998	Richter et al.
	4,891,225 A	1/1990 Langer et al.	5,833,694 A	11/1998	Poncet
	4,988,356 A	1/1991 Crittenden et al.	5,836,964 A	11/1998	Richter et al.
	4,994,066 A	2/1991 Voss	5,843,092 A	12/1998	Heller et al.
	4,994,069 A	2/1991 Ritchart et al.	5,855,563 A	1/1999	Kaplan et al.
	5,013,318 A	5/1991 Spranza, III	5,858,556 A	1/1999	Eckert et al.
	5,040,548 A	8/1991 Yock	5,870,381 A	2/1999	Kawasaki et al.
	5,064,435 A	11/1991 Porter	5,879,370 A	3/1999	Fischell et al.
	5,092,877 A	3/1992 Pinchuk	5,891,190 A	4/1999	Boneau
	5,102,417 A	4/1992 Palmaz	5,893,887 A	4/1999	Jayaraman
	5,104,404 A	4/1992 Wolff	5,895,398 A	4/1999	Wensel et al.
	5,122,154 A	6/1992 Rhodes	5,899,935 A	5/1999	Ding
	5,135,535 A	8/1992 Kramer	5,902,332 A	5/1999	Schatz
	5,195,984 A	3/1993 Schatz	5,911,754 A	6/1999	Kanesaka et al.
	5,217,495 A	6/1993 Kaplan et al.	5,919,175 A	7/1999	Sirhan
	5,219,355 A	6/1993 Parodi et al.	5,922,020 A	7/1999	Klein et al.
	5,226,913 A	7/1993 Pinchuk	5,961,536 A	10/1999	Mickley et al.
	5,246,421 A	9/1993 Saab	5,968,069 A	10/1999	Dusbabek et al.
	5,273,536 A	12/1993 Savas	5,972,027 A	10/1999	Johnson
	5,282,824 A	2/1994 Gianturco	5,976,107 A	11/1999	Mertens et al.
	5,300,085 A	4/1994 Yock	5,976,155 A	11/1999	Foreman et al.
	5,312,415 A	5/1994 Palermo	5,980,484 A	11/1999	Ressemann et al.
	5,334,187 A	8/1994 Fischell et al.	5,980,486 A	11/1999	Enger
	5,403,341 A	4/1995 Solar	5,980,514 A	11/1999	Kupiecki et al.
	5,421,955 A	6/1995 Lau et al.	5,980,552 A	11/1999	Pinchasik et al.
	5,456,694 A	10/1995 Marin et al.	5,984,957 A	11/1999	Laptewicz, Jr. et al.
	5,456,713 A	10/1995 Chuter	5,997,563 A	12/1999	Kretzers et al.
	5,458,615 A	10/1995 Klemm et al.	6,004,328 A	12/1999	Solar
	5,478,349 A	12/1995 Nicholas	6,007,517 A	12/1999	Anderson
	5,490,837 A	2/1996 Blaeser et al.	6,017,363 A	1/2000	Hojeibane
	5,496,346 A	3/1996 Horzewski et al.	6,022,359 A	2/2000	Frantzen
	5,501,227 A	3/1996 Yock	6,022,374 A	2/2000	Imran
	5,507,768 A	4/1996 Lau et al.	6,033,434 A	3/2000	Borghi
	5,507,771 A	4/1996 Gianturco	6,036,725 A	3/2000	Avellanet
	5,514,093 A	5/1996 Ellis et al.	6,039,721 A	3/2000	Johnson et al.
	5,514,154 A	5/1996 Lau et al.	6,042,589 A	3/2000	Marianne
	5,527,354 A	6/1996 Fontaine et al.	6,048,361 A	4/2000	Oopen
	5,549,551 A	8/1996 Peacock, III et al.	6,056,722 A	5/2000	Jayaraman
	5,549,563 A	8/1996 Kronner	6,056,775 A	5/2000	Borghi et al.
	5,549,635 A	8/1996 Solar	6,059,811 A	5/2000	Pinchasik et al.
	5,554,181 A	9/1996 Das	6,059,824 A	5/2000	Taheri
	5,562,725 A	10/1996 Schmitt et al.	6,066,155 A	5/2000	Amann et al.
	5,571,086 A	11/1996 Kaplan et al.	6,068,655 A	5/2000	Seguin et al.
	5,593,412 A	1/1997 Martinez et al.	6,070,589 A	6/2000	Keith et al.
	5,607,444 A	3/1997 Lam	6,086,604 A	7/2000	Fischell et al.
	5,607,463 A	3/1997 Schwartz et al.	6,090,063 A	7/2000	Makower et al.
	5,609,627 A	3/1997 Goicoechea et al.			
	5,628,775 A	5/1997 Jackson et al.			

(56)

References Cited

U.S. PATENT DOCUMENTS

6,090,136 A	7/2000	McDonald et al.	6,527,789 B1	3/2003	Lau et al.
6,096,071 A	8/2000	Yadav	6,527,799 B2	3/2003	Shanley
6,096,073 A	8/2000	Webster et al.	6,530,944 B2	3/2003	West et al.
6,099,497 A	8/2000	Adams et al.	6,540,777 B2	4/2003	Stenzel
6,102,942 A	8/2000	Ahari	6,540,779 B2	4/2003	Richter et al.
6,106,530 A	8/2000	Harada	6,551,350 B1	4/2003	Thornton et al.
RE36,857 E	9/2000	Euteneuer et al.	6,555,157 B1	4/2003	Hossainy
6,117,117 A	9/2000	Mauch	6,569,180 B1	5/2003	Sirhan et al.
6,120,522 A	9/2000	Vrba et al.	6,575,993 B1	6/2003	Yock
6,123,712 A	9/2000	Di Caprio et al.	6,579,305 B1	6/2003	Lashinski
6,123,723 A	9/2000	Konya et al.	6,579,309 B1	6/2003	Loos et al.
6,126,685 A	10/2000	Lenker et al.	6,582,394 B1	6/2003	Reiss et al.
6,129,738 A	10/2000	Lashinski et al.	6,582,460 B1	6/2003	Cryer
6,129,756 A	10/2000	Kugler	6,585,756 B1	7/2003	Strecker
6,132,460 A	10/2000	Thompson	6,592,549 B2	7/2003	Gerdts et al.
6,142,973 A	11/2000	Carleton et al.	6,596,020 B2	7/2003	Vardi et al.
6,143,016 A	11/2000	Bleam et al.	6,596,022 B2	7/2003	Lau et al.
6,165,167 A	12/2000	Delaloye	6,599,296 B1	7/2003	Gillick et al.
6,165,210 A	12/2000	Lau et al.	6,599,314 B2	7/2003	Mathis
6,179,878 B1	1/2001	Duering	6,602,282 B1	8/2003	Yan
6,183,509 B1	2/2001	Dibie	6,605,062 B1	8/2003	Hurley et al.
6,187,034 B1	2/2001	Frantzen	6,605,109 B2	8/2003	Fiedler
6,190,402 B1	2/2001	Horton et al.	6,607,553 B1	8/2003	Healy et al.
6,196,995 B1	3/2001	Fagan	6,645,517 B2	11/2003	West
6,200,337 B1	3/2001	Moriuchi et al.	6,645,547 B1	11/2003	Shekalim et al.
6,210,429 B1	4/2001	Vardi et al.	6,656,212 B2	12/2003	Ravenscroft et al.
6,238,991 B1	5/2001	Suzuki	6,660,031 B2	12/2003	Tran et al.
6,241,691 B1	6/2001	Ferrera et al.	6,660,381 B2	12/2003	Halas et al.
6,251,132 B1	6/2001	Ravenscroft et al.	6,666,883 B1	12/2003	Seguin et al.
6,251,134 B1	6/2001	Alt et al.	6,676,695 B2	1/2004	Solem
6,254,612 B1	7/2001	Hieshima	6,679,909 B2	1/2004	McIntosh et al.
6,254,628 B1	7/2001	Wallace et al.	6,685,721 B1	2/2004	Kramer
6,258,117 B1	7/2001	Camrud et al.	6,685,730 B2	2/2004	West et al.
6,264,682 B1	7/2001	Wilson et al.	6,689,156 B1	2/2004	Davidson et al.
6,264,688 B1	7/2001	Herklotz et al.	6,692,465 B2	2/2004	Kramer
6,267,783 B1	7/2001	Letendre et al.	6,692,483 B2	2/2004	Vardi et al.
6,273,895 B1	8/2001	Pinchuk et al.	6,699,280 B2	3/2004	Camrud et al.
6,273,911 B1	8/2001	Cox et al.	6,699,724 B1	3/2004	West et al.
6,273,913 B1	8/2001	Wright et al.	6,702,843 B1	3/2004	Brown
6,312,458 B1	11/2001	Golds	6,706,062 B2	3/2004	Vardi et al.
6,315,794 B1	11/2001	Richter	6,709,379 B1	3/2004	Brandau et al.
6,319,277 B1	11/2001	Rudnick et al.	6,709,440 B2	3/2004	Callol et al.
6,322,586 B1	11/2001	Monroe et al.	6,712,827 B2	3/2004	Ellis et al.
6,325,823 B1	12/2001	Horzewski et al.	6,712,845 B2	3/2004	Hossainy
6,325,826 B1	12/2001	Vardi et al.	6,723,071 B2	4/2004	Gerdts et al.
6,334,871 B1	1/2002	Dor et al.	6,736,842 B2	5/2004	Healy et al.
6,344,053 B1	2/2002	Boneau	6,749,628 B1	6/2004	Callol et al.
6,344,056 B1	2/2002	Dehdashtian	6,761,734 B2	7/2004	Suhr
6,344,272 B1	2/2002	Oldenburg et al.	6,770,091 B2	8/2004	Richter et al.
6,357,104 B1	3/2002	Myers	6,778,316 B2	8/2004	Halas et al.
6,361,555 B1	3/2002	Wilson	6,800,065 B2	10/2004	Duane et al.
6,375,676 B1	4/2002	Cox	6,811,566 B1	11/2004	Penn et al.
6,379,365 B1	4/2002	Diaz	6,825,203 B2	11/2004	Pasternak et al.
6,383,171 B1	5/2002	Gifford et al.	6,835,203 B1	12/2004	Vardi et al.
6,398,807 B1	6/2002	Chouinard et al.	6,837,901 B2	1/2005	Rabkin et al.
6,409,753 B1	6/2002	Brown et al.	6,849,084 B2	2/2005	Rabkin et al.
6,415,696 B1	7/2002	Erickeson et al.	6,852,252 B2	2/2005	Halas et al.
6,419,693 B1	7/2002	Fariabi	6,855,125 B2	2/2005	Shanley
6,428,811 B1	8/2002	West et al.	6,858,034 B1	2/2005	Hijlkema et al.
6,443,982 B1	9/2002	Israel et al.	6,875,228 B2	4/2005	Pinchasik et al.
6,451,025 B1	9/2002	Jervis	6,878,161 B2	4/2005	Lenker
6,451,050 B1	9/2002	Rudakov et al.	6,879,370 B2	4/2005	Yokoue et al.
6,464,720 B2	10/2002	Boatman et al.	6,884,258 B2	4/2005	Vardi et al.
6,468,298 B1	10/2002	Pelton	6,893,417 B2	5/2005	Gribbons et al.
6,468,299 B2	10/2002	Stack et al.	6,896,695 B2	5/2005	Mueller et al.
6,485,510 B1	11/2002	Camrud et al.	6,908,477 B2	6/2005	McGuckin, Jr. et al.
6,485,511 B2	11/2002	Lau et al.	6,918,928 B2	7/2005	Wolinsky et al.
6,488,694 B1	12/2002	Lau et al.	6,939,376 B2	9/2005	Shulz et al.
6,488,702 B1	12/2002	Besselink	6,945,989 B1	9/2005	Betelia et al.
6,488,703 B1	12/2002	Kveen et al.	6,945,995 B2	9/2005	Nicholas
6,511,468 B1	1/2003	Cragg et al.	6,949,120 B2	9/2005	Kveen et al.
6,514,281 B1	2/2003	Blaeser et al.	6,951,053 B2	10/2005	Padilla et al.
6,520,986 B2	2/2003	Martin et al.	6,955,687 B2	10/2005	Richter et al.
6,520,987 B1	2/2003	Plante	6,955,688 B2	10/2005	Wilson et al.
6,520,988 B1	2/2003	Colombo et al.	6,962,602 B2	11/2005	Vardi et al.
			6,989,026 B2	1/2006	Richter et al.
			7,005,454 B2	2/2006	Brocchini et al.
			7,037,327 B2	5/2006	Salmon et al.
			7,090,694 B1	8/2006	Morris et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,101,840 B2	9/2006	Brocchini et al.	2003/0139797 A1	7/2003	Johnson et al.
7,137,993 B2	11/2006	Acosta et al.	2003/0139798 A1	7/2003	Brown et al.
7,147,655 B2	12/2006	Chermoni	2003/0163085 A1	8/2003	Tanner et al.
7,147,656 B2	12/2006	Andreas et al.	2003/0176909 A1	9/2003	Kusleika
7,182,779 B2	2/2007	Acosta et al.	2003/0191516 A1	10/2003	Weldon et al.
7,192,440 B2	3/2007	Andreas et al.	2003/0192164 A1	10/2003	Austin
7,220,275 B2	5/2007	Davidson et al.	2003/0195609 A1	10/2003	Berenstein
7,241,308 B2	7/2007	Andreas et al.	2003/0199821 A1	10/2003	Gerdts et al.
7,270,668 B2	9/2007	Andreas et al.	2003/0204238 A1	10/2003	Tedeschi
7,294,146 B2	11/2007	Chew et al.	2003/0212447 A1	11/2003	Euteneuer
7,300,456 B2	11/2007	Andreas et al.	2003/0225446 A1	12/2003	Hartley
7,309,350 B2	12/2007	Landreville et al.	2004/0024450 A1	2/2004	Shulze et al.
7,314,480 B2	1/2008	Eidenschink et al.	2004/0030380 A1	2/2004	Shulze et al.
7,320,702 B2	1/2008	Hammersmark et al.	2004/0044395 A1	3/2004	Nelson
7,323,006 B2	1/2008	Andreas et al.	2004/0044398 A1	3/2004	Nicholas
7,323,009 B2	1/2008	Suhr et al.	2004/0087965 A1	5/2004	Levine et al.
7,326,236 B2	2/2008	Andreas et al.	2004/0093061 A1	5/2004	Acosta et al.
7,326,242 B2	2/2008	Eidenschink	2004/0093067 A1	5/2004	Israel
7,341,598 B2	3/2008	Davidson et al.	2004/0093077 A1	5/2004	White et al.
7,344,556 B2 *	3/2008	Seguin A61F 2/915 623/1.11	2004/0098081 A1	5/2004	Landreville et al.
7,387,639 B2	6/2008	Bourang et al.	2004/0106979 A1	6/2004	Goicoechea
7,445,688 B2	11/2008	Suzuki et al.	2004/0111145 A1	6/2004	Serino et al.
7,520,895 B2	4/2009	Douglas et al.	2004/0117008 A1	6/2004	Wnendt et al.
7,537,609 B2	5/2009	Davidson et al.	2004/0176832 A1	9/2004	Hartley et al.
7,540,881 B2	6/2009	Meyer et al.	2004/0186551 A1	9/2004	Kao et al.
7,635,383 B2	12/2009	Gumm	2004/0193245 A1	9/2004	Deem et al.
7,641,684 B2	1/2010	Hilaire et al.	2004/0215165 A1	10/2004	Coyle et al.
7,641,685 B2	1/2010	Richter	2004/0215312 A1	10/2004	Andreas et al.
7,695,508 B2	4/2010	Der Leest et al.	2004/0243217 A1	12/2004	Andersen et al.
8,016,870 B2	9/2011	Chew et al.	2004/0249434 A1	12/2004	Andreas et al.
8,070,789 B2	12/2011	Will et al.	2004/0249435 A1	12/2004	Andreas et al.
8,769,796 B2	7/2014	Bourang et al.	2005/0010276 A1	1/2005	Acosta et al.
8,795,347 B2	8/2014	Bourang et al.	2005/0038505 A1	2/2005	Shuize et al.
8,808,347 B2	8/2014	Bourang et al.	2005/0049673 A1	3/2005	Andreas et al.
8,821,562 B2	9/2014	Bourang et al.	2005/0049680 A1	3/2005	Fischell et al.
8,828,071 B2	9/2014	Bourang et al.	2005/0080474 A1	4/2005	Andreas et al.
8,979,917 B2	3/2015	Bourang et al.	2005/0080475 A1	4/2005	Andreas et al.
2001/0003161 A1	6/2001	Vardi et al.	2005/0085845 A1	4/2005	Hilaire et al.
2001/0020154 A1	9/2001	Bigus et al.	2005/0090846 A1	4/2005	Pedersen et al.
2001/0020181 A1	9/2001	Layne	2005/0101624 A1	5/2005	Betts et al.
2001/0044595 A1	11/2001	Reydel et al.	2005/0125051 A1	6/2005	Eidenschink et al.
2001/0044622 A1	11/2001	Vardi et al.	2005/0131008 A1	6/2005	Betts et al.
2001/0044632 A1	11/2001	Daniel et al.	2005/0133164 A1	6/2005	Fischer et al.
2001/0049547 A1	12/2001	Moore	2005/0143827 A1	6/2005	Globerman et al.
2002/0037358 A1	3/2002	Barry et al.	2005/0149159 A1	7/2005	Andreas et al.
2002/0091439 A1	7/2002	Baker et al.	2005/0165378 A1	7/2005	Heinrich et al.
2002/0107560 A1	8/2002	Richter	2005/0182473 A1	8/2005	Eidenschink et al.
2002/0111671 A1	8/2002	Stenzel	2005/0183259 A1	8/2005	Eidenschink et al.
2002/0128706 A1	9/2002	Osypka	2005/0197688 A1	9/2005	Theron et al.
2002/0138132 A1	9/2002	Brown	2005/0209674 A1	9/2005	Kutscher et al.
2002/0143382 A1	10/2002	Hijlkema et al.	2005/0222671 A1	10/2005	Schaeffer et al.
2002/0151924 A1	10/2002	Shiber	2005/0228477 A1	10/2005	Grainger et al.
2002/0151955 A1	10/2002	Tran et al.	2005/0245637 A1	11/2005	Hossainy et al.
2002/0156496 A1	10/2002	Chermoni	2005/0288763 A1	12/2005	Andreas et al.
2002/0173835 A1	11/2002	Bourang et al.	2005/0288764 A1	12/2005	Snow et al.
2002/0177890 A1	11/2002	Lenker	2005/0288766 A1	12/2005	Plain et al.
2002/0183763 A1	12/2002	Callol et al.	2006/0069424 A1	3/2006	Acosta et al.
2002/0188343 A1	12/2002	Mathis	2006/0100694 A1	5/2006	Globerman
2002/0188347 A1	12/2002	Mathis	2006/0123874 A1	6/2006	Motsenbocker
2002/0193873 A1	12/2002	Brucker et al.	2006/0200223 A1	9/2006	Andreas et al.
2003/0028233 A1	2/2003	Vardi et al.	2006/0206190 A1	9/2006	Chermoni
2003/0029039 A1	2/2003	Richter et al.	2006/0229700 A1	10/2006	Acosta et al.
2003/0045923 A1	3/2003	Bashiri et al.	2006/0229706 A1	10/2006	Shulze et al.
2003/0093143 A1	5/2003	Zhao et al.	2006/0271090 A1 *	11/2006	Shaked et al. 606/192
2003/0097169 A1	5/2003	Brucker et al.	2006/0271150 A1	11/2006	Andreas et al.
2003/0114912 A1	6/2003	Sequin et al.	2006/0271151 A1	11/2006	McGarry et al.
2003/0114919 A1	6/2003	McQuiston et al.	2006/0282147 A1	12/2006	Andreas et al.
2003/0114922 A1	6/2003	Iwasaka et al.	2006/0282149 A1	12/2006	Kao
2003/0125791 A1	7/2003	Sequin et al.	2006/0282150 A1	12/2006	Olson et al.
2003/0125800 A1	7/2003	Shulze et al.	2006/0287726 A1	12/2006	Segal et al.
2003/0125802 A1	7/2003	Callol et al.	2007/0027521 A1	2/2007	Andreas et al.
2003/0135259 A1	7/2003	Simso	2007/0027524 A1	2/2007	Johnson et al.
2003/0135266 A1	7/2003	Chew et al.	2007/0055351 A1	3/2007	Eidenschink et al.
2003/0139796 A1	7/2003	Sequin et al.	2007/0061003 A1	3/2007	Shmulewitz et al.
			2007/0067012 A1	3/2007	George et al.
			2007/0088368 A1	4/2007	Acosta et al.
			2007/0088420 A1	4/2007	Andreas et al.
			2007/0088422 A1	4/2007	Chew et al.
			2007/0100423 A1	5/2007	Acosta et al.

(56)

References Cited

FOREIGN PATENT DOCUMENTS

U.S. PATENT DOCUMENTS					
2007/0100424	A1	5/2007	Chew et al.	CN	101035488 A 12/2007
2007/0106365	A1	5/2007	Andreas et al.	CN	102215780 A 10/2011
2007/0118202	A1	5/2007	Chermoni	CN	103037813 A 4/2013
2007/0118203	A1	5/2007	Chermoni	CN	103037815 A 4/2013
2007/0118204	A1	5/2007	Chermoni	CN	103037816 A 4/2013
2007/0129733	A1	6/2007	Will et al.	CN	103037817 A 4/2013
2007/0156225	A1	7/2007	George et al.	CN	103068345 A 4/2013
2007/0156226	A1	7/2007	Chew et al.	EP	0 203 945 B2 12/1986
2007/0179587	A1	8/2007	Acosta et al.	EP	0 274 129 B1 7/1988
2007/0203571	A1	8/2007	Kaplan et al.	EP	0 282 143 A1 9/1988
2007/0219611	A1	9/2007	Krever et al.	EP	0 505 686 A1 9/1992
2007/0219612	A1	9/2007	Andreas et al.	EP	0 533 960 A1 3/1993
2007/0219613	A1	9/2007	Kao et al.	EP	0 714 640 A1 6/1996
2007/0219625	A1	9/2007	Venturelli et al.	EP	0 596 145 A1 5/1997
2007/0265637	A1	11/2007	Andreas et al.	EP	0 897 700 A1 2/1999
2007/0270936	A1	11/2007	Andreas et al.	EP	0 947 180 A2 10/1999
2007/0276460	A1	11/2007	Davis et al.	EP	1 258 230 A2 11/2002
2007/0276461	A1	11/2007	Andreas et al.	EP	1 277 449 A1 1/2003
2007/0281117	A1	12/2007	Kaplan et al.	EP	1 523 959 A2 4/2005
2007/0282419	A1	12/2007	Hilaire et al.	EP	1 523 960 A2 4/2005
2007/0292518	A1	12/2007	Ludwig	EP	1 266 638 A2 10/2005
2008/0009932	A1	1/2008	Ta et al.	EP	1788977 B1 3/2008
2008/0009933	A1	1/2008	Ta et al.	EP	1 905 398 A2 4/2008
2008/0051869	A1	2/2008	Yribarren	EP	2344068 A1 7/2011
2008/0071345	A1	3/2008	Hammersmark et al.	EP	2549949 A1 1/2013
2008/0077229	A1	3/2008	Andreas et al.	EP	2549950 A1 1/2013
2008/0091257	A1	4/2008	Andreas et al.	EP	2549951 A1 1/2013
2008/0097299	A1	4/2008	Andreas et al.	EP	2549952 A1 1/2013
2008/0097574	A1	4/2008	Andreas et al.	EP	2549958 A1 1/2013
2008/0132989	A1	6/2008	Snow et al.	EP	2 672 925 12/2013
2008/0147162	A1	6/2008	Andreas et al.	EP	2 672 932 12/2013
2008/0199510	A1	8/2008	Ruane et al.	JP	10-043313 2/1998
2008/0208309	A1	8/2008	Saeed	JP	2003-532437 A 11/2003
2008/0208311	A1	8/2008	Kao et al.	JP	2004-528877 A 9/2004
2008/0208318	A1	8/2008	Kao et al.	JP	2007-508082 A 4/2007
2008/0221655	A1	9/2008	Miller	JP	2010-503465 A 4/2010
2008/0234795	A1	9/2008	Snow et al.	JP	2012503534 A 2/2012
2008/0234798	A1	9/2008	Chew et al.	JP	2013523215 A 6/2013
2008/0234799	A1	9/2008	Acosta et al.	WO	96/26689 A1 9/1996
2008/0269865	A1	10/2008	Snow et al.	WO	96/33677 A2 10/1996
2009/0076584	A1	3/2009	Mao et al.	WO	97/46174 A1 12/1997
2009/0105686	A1	4/2009	Snow et al.	WO	97/48351 A1 12/1997
2009/0132019	A1	5/2009	Duffy et al.	WO	98/20810 A1 5/1998
2009/0143854	A1	6/2009	Adams et al.	WO	98/37833 A1 9/1998
2009/0171430	A1	7/2009	Baim et al.	WO	98/58600 A1 12/1998
2009/0182270	A1	7/2009	Nanavati	WO	99/01087 A1 1/1999
2009/0228088	A1	9/2009	Lowe et al.	WO	00/12832 A2 3/2000
2009/0240321	A1	9/2009	Davidson et al.	WO	00/15151 A1 3/2000
2009/0254167	A1	10/2009	Ricci et al.	WO	00/25841 A1 5/2000
2009/0259285	A1	10/2009	Duane et al.	WO	00/32136 A1 6/2000
2009/0287289	A1	11/2009	Sagedahl et al.	WO	00/41649 A1 7/2000
2009/0299454	A1	12/2009	Jennings et al.	WO	00/50116 A1 8/2000
2009/0319030	A1	12/2009	Yadin et al.	WO	00/62708 A1 10/2000
2009/0326641	A1	12/2009	Davis et al.	WO	00/72780 A1 12/2000
2010/0004737	A1	1/2010	Eidenschink	WO	00/74595 A1 12/2000
2010/0030183	A1	2/2010	Toner et al.	WO	01/70297 A2 9/2001
2010/0036477	A1	2/2010	Bronson et al.	WO	01/91918 A1 12/2001
2010/0042199	A1	2/2010	Burton	WO	02/060344 A2 8/2002
2010/0049298	A1	2/2010	Hamer et al.	WO	02/085253 A1 10/2002
2010/0057020	A1	3/2010	Uretsky	WO	03/022178 A1 3/2003
2010/0063571	A1	3/2010	Roach et al.	WO	03/047651 A2 6/2003
2010/0106238	A1	4/2010	Hilaire et al.	WO	03/051425 A2 6/2003
2011/0029061	A1	2/2011	Ahn et al.	WO	03/055414 7/2003
2011/0282427	A1	11/2011	Bourang et al.	WO	03/105922 A2 12/2003
2011/0307044	A1	12/2011	Bourang et al.	WO	2004/017865 A1 3/2004
2011/0307045	A1	12/2011	Bourang et al.	WO	2004/043299 A1 5/2004
2011/0307046	A1	12/2011	Bourang et al.	WO	2004/043301 A1 5/2004
2011/0307047	A1	12/2011	Bourang et al.	WO	2004/043410 A1 5/2004
2011/0307052	A1	12/2011	Bourang et al.	WO	2004/052237 A2 6/2004
2014/0100647	A1	4/2014	Bourang	WO	2005/013853 A2 2/2005
2015/0032196	A1	1/2015	Bourang et al.	WO	2005/039681 A1 5/2005
				WO	2006/036939 A2 4/2006
				WO	2006/047520 A2 5/2006
				WO	2007/035805 A2 3/2007
				WO	2007/053187 A2 5/2007
				WO	2007/146411 A2 12/2007
				WO	2008/005111 A1 1/2008

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 2008/033621	A1	3/2008
WO	WO 2008/130503	A2	10/2008
WO	WO 2009/148594	A1	12/2009
WO	2010/036982	A1	4/2010
WO	WO 2010/036982	A1	4/2010
WO	2011/119879	A1	9/2011
WO	2011/119880	A1	9/2011
WO	2011/119882	A1	9/2011
WO	2011/119883	A1	9/2011
WO	2011/119884	A1	9/2011
WO	2012/109365	A1	8/2012
WO	2012/109382	A2	8/2012

OTHER PUBLICATIONS

English Translation and Second Office Action for corresponding Chinese Patent Application No. 200980143592.X dated Apr. 21, 2014, 26 pages.

U.S. Appl. No. 14/621,231, filed Feb. 12, 2015 by Bourang et al. (Unpublished.).

U.S. Appl. No. 14/317,387, filed Jun. 27, 2014 by Bourang et al. (Unpublished.).

U.S. Appl. No. 14/294,631, filed Jun. 3, 2014 by Bourang et al. (Unpublished.).

U.S. Appl. No. 14/314,361, filed Jun. 25, 2014 by Bourang et al. (Unpublished.).

U.S. Appl. No. 14/313,742, filed Jun. 24, 2014 by Bourang et al. (Unpublished.).

U.S. Appl. No. 14/321,506, filed Jul. 1, 2014 by Bourang et al. (Unpublished.).

“Drug Delivery Stent With Holes Located on Neutral Axis”; No. 429007; Research Disclosure, Kenneth Mason Publications, Hampshire, CB; Jan. 2000; pp. 13; vol. 2266.

“Stent”. Definitions from Dictionary.com. Unabridged (v1.01). Retrieved Sep. 22, 2006, from Dictionary.com, located at <http://dictionary.reference.com/search?q=stent>; 1 page.

Colombo, “The InVatec Bifurcation Stent Solution” Bifurcation Stents: Novel Solutions, TCT 2003, Washington: Sep. 15-19, 2003, 24 pages.

Cooley, Patrick et al.; “Applications of Ink-Jet Printing Technology to BioMEMs and Microfluidic Systems”; Proceedings, SPIE Conference on Microfluidics and BioMEMs; Oct. 2001; 12 pages.

Evans Analytical Group; “Functional Sites on Non-polymeric Materials: Gas Plasma Treatment and Surface Analysis”; located at <http://www.eaglabs.com>; 2003; 2 pages.

International Search Report mailed on May 27, 2011, for PCT Patent Application No. PCT/US2011/029863, filed on Mar. 24, 2011, 2 pages.

Joung, Yoon Ki et al.; “Estrogen Release from Metallic Stent Surface for the Prevention of Restenosis”; Journal of Controlled Release; 2003; pp. 83-91; vol. 92.

Lefèvre, Thierry et al. “Approach to Coronary Bifurcation Stenting in 2003”; Euro PCR; May 2003; pp. 127-154.

Stimpson, Donald I. et al; “Parallel Production of Oligonucleotide Arrays Using Membranes and Reagent Jet Printing”; BioTechniques; Nov. 1998; pp. 886-890; vol. 25.

Supplementary European Search Report dated Mar. 25, 2008, for EP Patent Application No. 05727731.1, 2 pages.

Supplementary European Search Report mailed on Apr. 9, 2008, for EP Patent Application No. 05744136.2, 3 pages.

U.S. Appl. No. 09/097,855, filed Jun. 15, 1998, first named inventor: Enrique J. Klein.

U.S. Appl. No. 09/225,364, filed Jan. 4, 1999, first named inventor: Aaron V. Kaplan.

U.S. Appl. No. 10/874,859, filed Jun. 22, 2004, first named inventor: Pablo Acosta.

U.S. Appl. No. 60/336,607, filed Dec. 3, 2001, first named inventor: Bernard Andreas.

U.S. Appl. No. 60/336,767, filed Dec. 3, 2001, first named inventor: Bernard Andreas.

U.S. Appl. No. 60/336,967, filed Dec. 3, 2001, first named inventor: Sunmi Chew.

U.S. Appl. No. 60/364,389, filed Mar. 13, 2002, first named inventor: Sunmi Chew.

U.S. Appl. No. 60/440,839, filed Jan. 17, 2003, first named inventor: Bernard Andreas.

U.S. Appl. No. 60/561,041, filed Apr. 9, 2004, first named inventor: Jeffry Grainger.

U.S. Appl. No. 60/784,309, filed Mar. 20, 2006, first named inventor: Bernard Andreas.

U.S. Appl. No. 60/810,522, filed Jun. 2, 2006, first named inventor: Stephen Kaplan.

U.S. Appl. No. 60/890,703, filed Feb. 20, 2007, first named inventor: Patrick Ruane.

U.S. Appl. No. 61/012,317, filed Dec. 7, 2007, first named inventor: Patrick Ruane.

Written Opinion of the International Searching Authority mailed on May 27, 2011, for PCT Patent Application No. PCT/US2011/029863, filed on Mar. 24, 2011, 11 pages.

First Office Action of Application No. CN 200980143592.X, Jun. 4, 2013, 10 pages.

International Preliminary Report on Patentability of Application No. PCT/US2009/058505, Oct. 28, 2010, 38 pages.

International Search Report and Written Opinion of Application No. PCT/US2009/058505, Nov. 25, 2009, 11 pages.

International Search Report and Written Opinion of Application No. PCT/US2011/029858, May 25, 2011, 10 pages.

International Preliminary Report on Patentability of Application No. PCT/US2011/029859, Sep. 25, 2012, 8 pages.

International Search Report and Written Opinion of Application No. PCT/US2011/029859, May 23, 2011, 8 pages.

International Preliminary Report on Patentability of Application No. PCT/US2011/029861, Sep. 25, 2012, 9 pages.

International Search Report and Written Opinion of Application No. PCT/US2011/029861, May 20, 2011, 11 pages.

International Preliminary Report on Patentability of Application No. PCT/US2011/029862, Sep. 25, 2012, 11 pages.

International Search Report and Written Opinion of Application No. PCT/US2011/029862, May 25, 2011, 13 pages.

International Preliminary Report on Patentability of Application No. PCT/US2011/029863, Sep. 25, 2012, 13 pages.

International Preliminary Report on Patentability of Application No. PCT/US2012/024347, Aug. 13, 2013, 8 pages.

International Search Report and Written Opinion of Application No. PCT/US2012/024347, Jun. 29, 2012, 13 pages.

International Preliminary Report on Patentability of Application No. PCT/US2012/024366, Aug. 13, 2013, 19 pages.

International Search Report and Written Opinion of Application No. PCT/US2012/024366, Sep. 7, 2012, 23 pages.

Invitation to Pay Additional Fees of Application No. PCT/US2012/024366, Jun. 1, 2012, 3 pages.

* cited by examiner

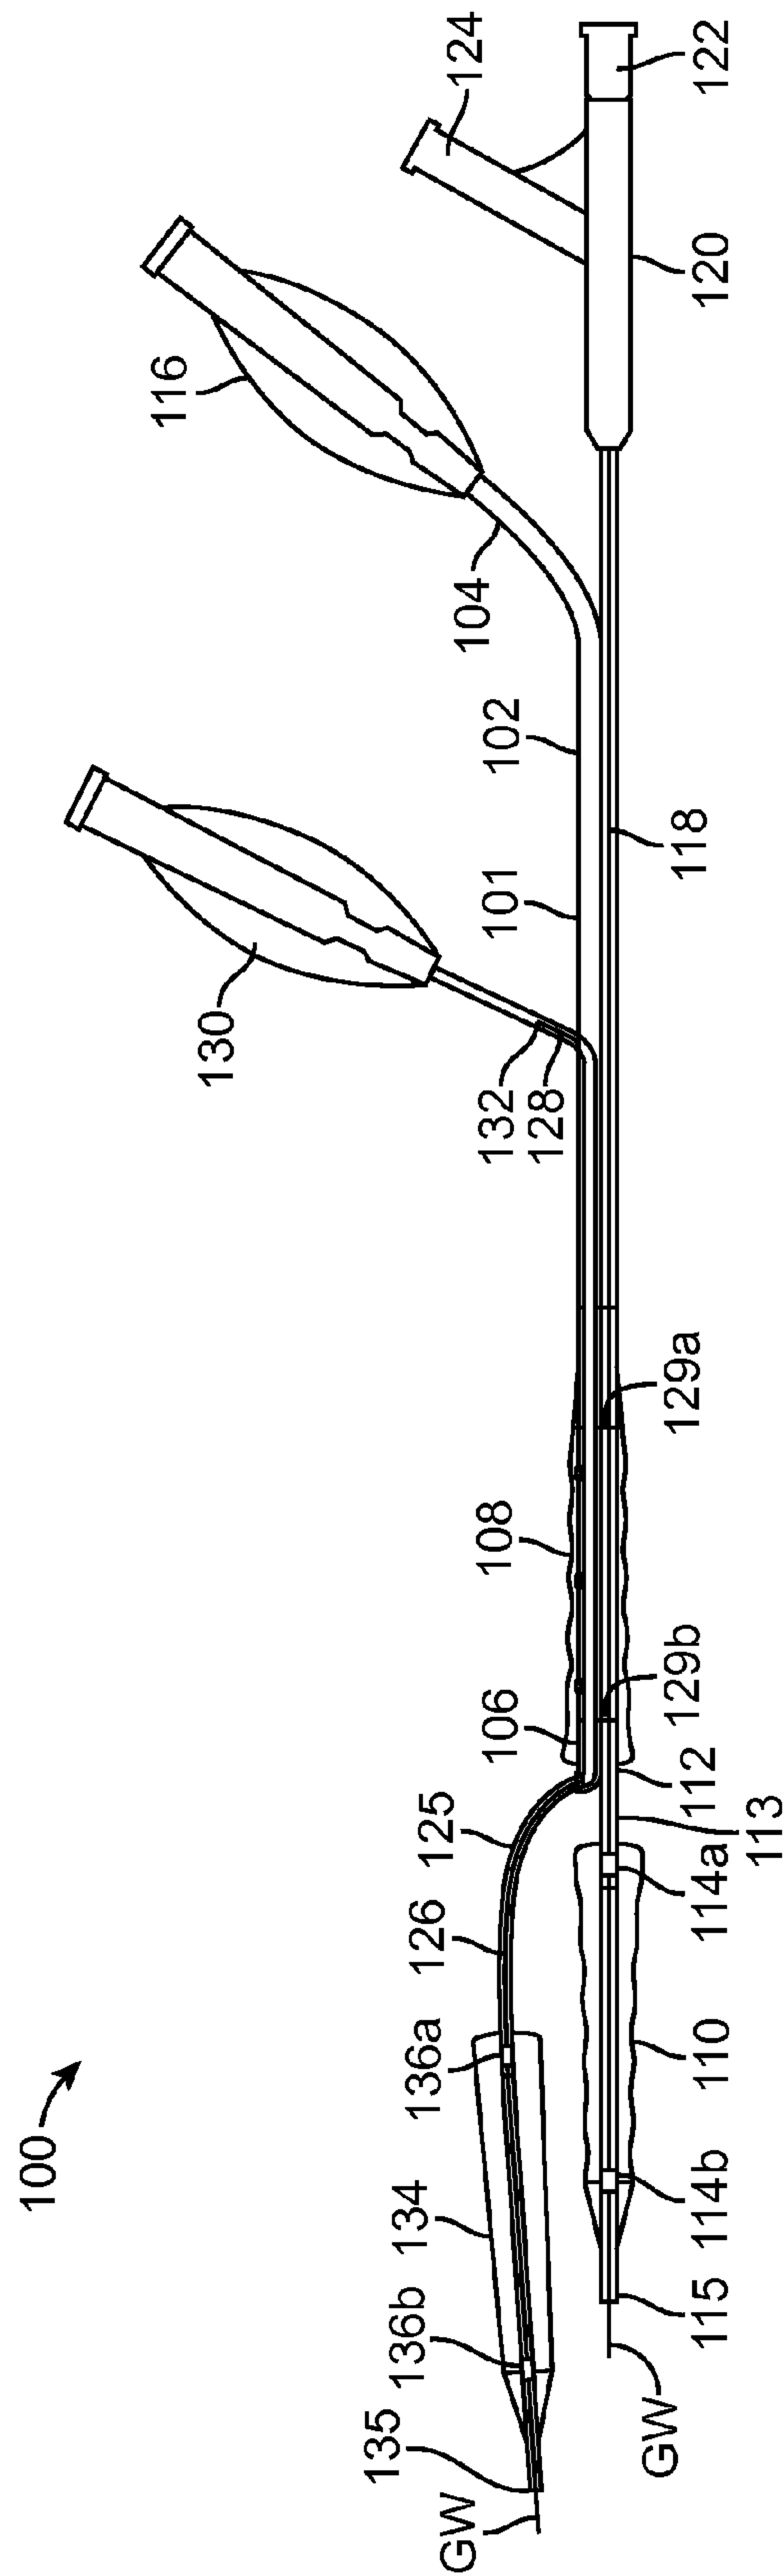


FIG. 1

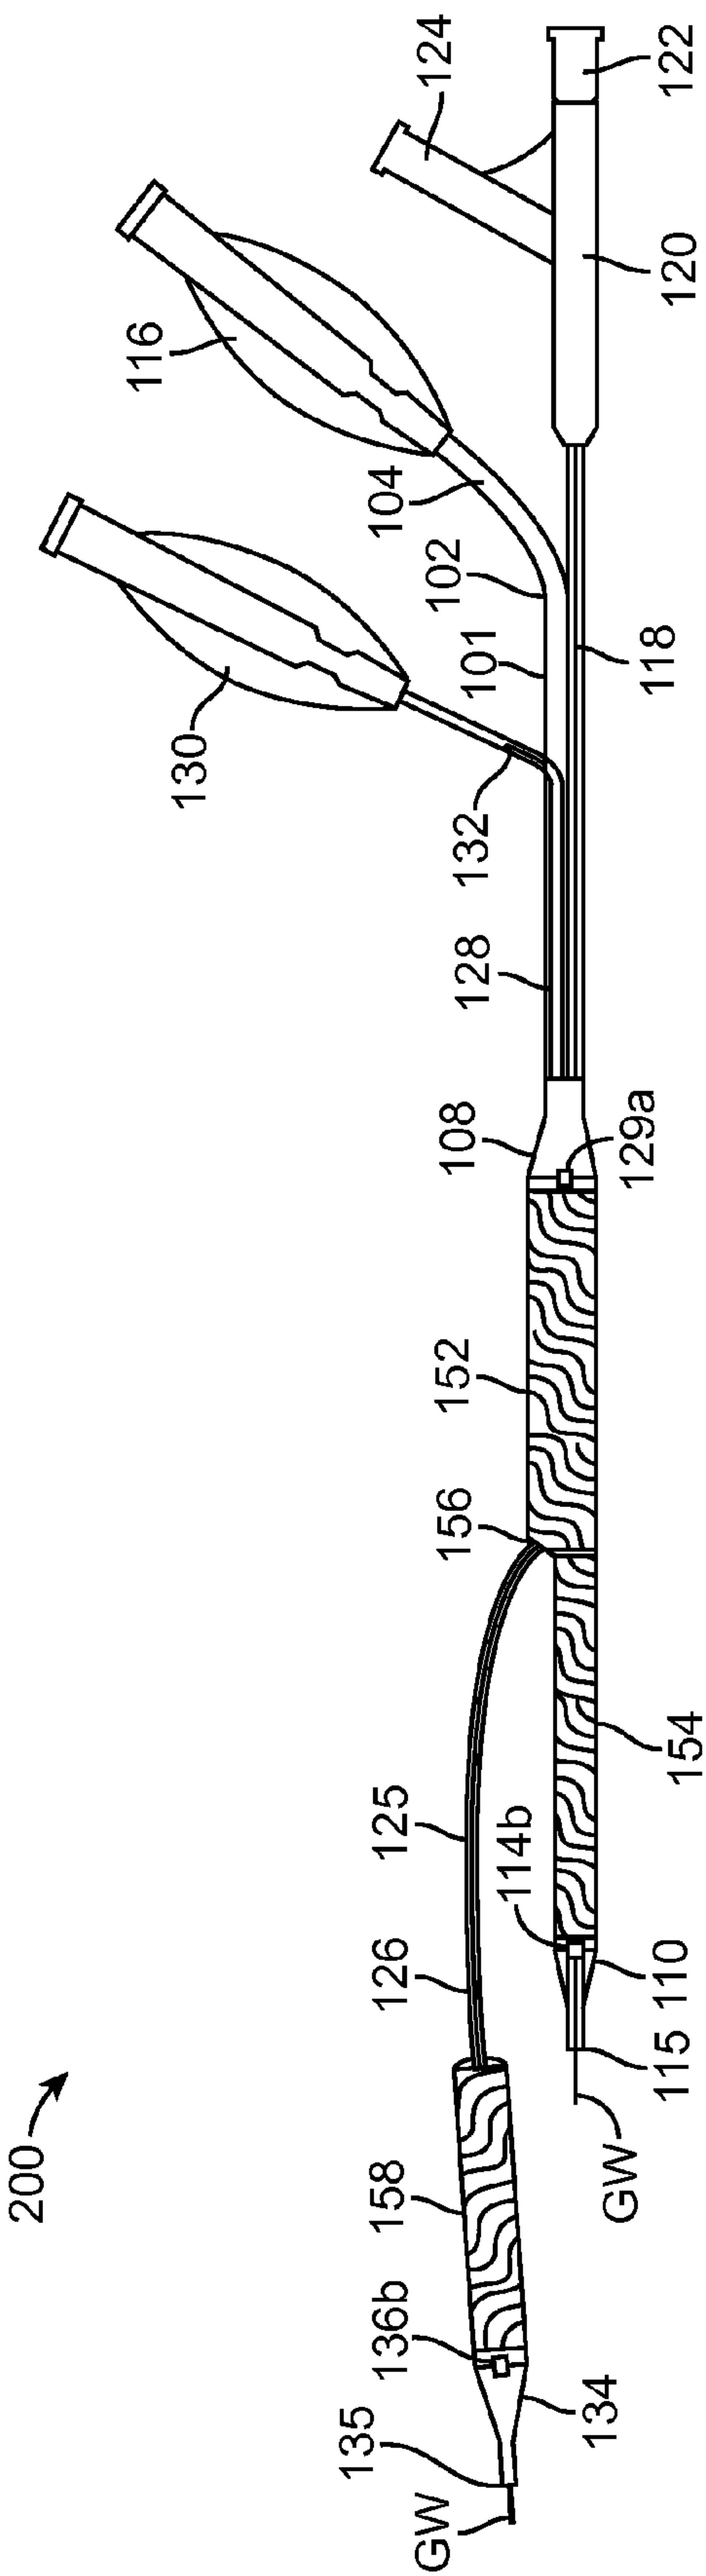


FIG. 2

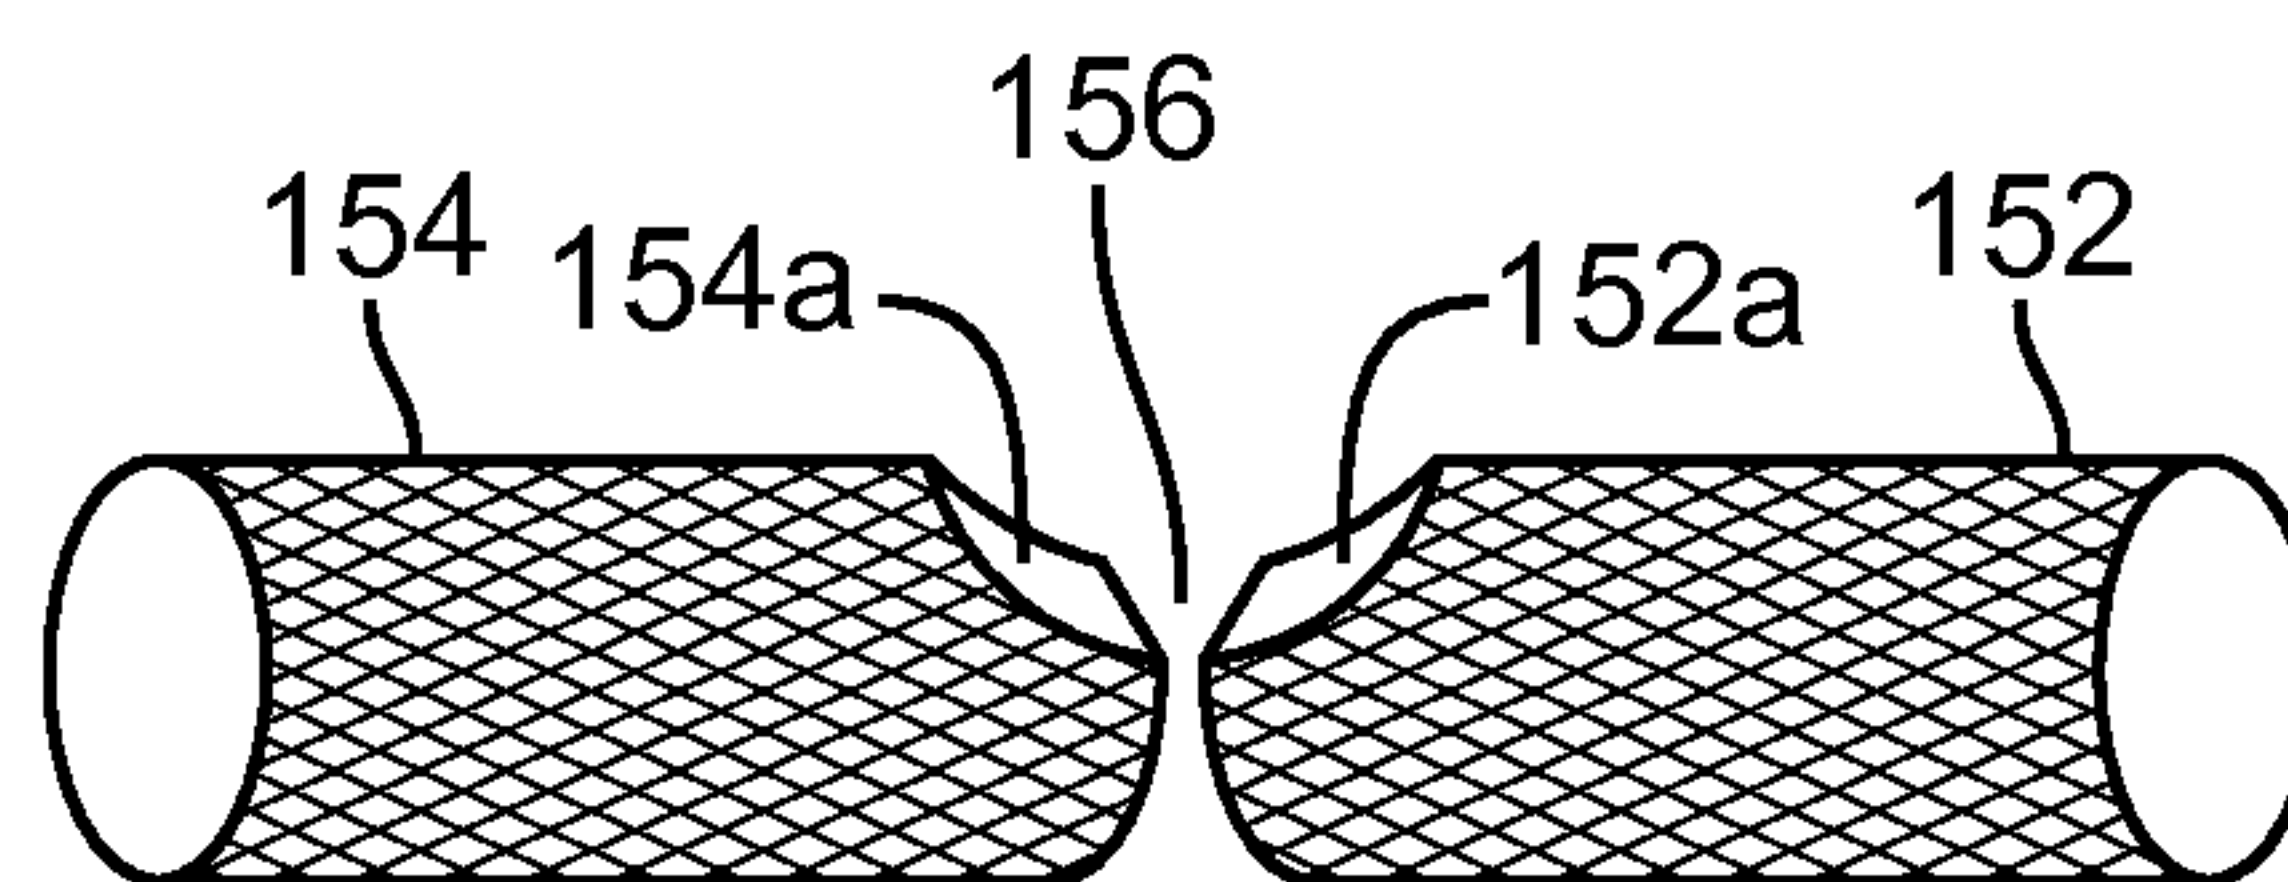


FIG. 3A

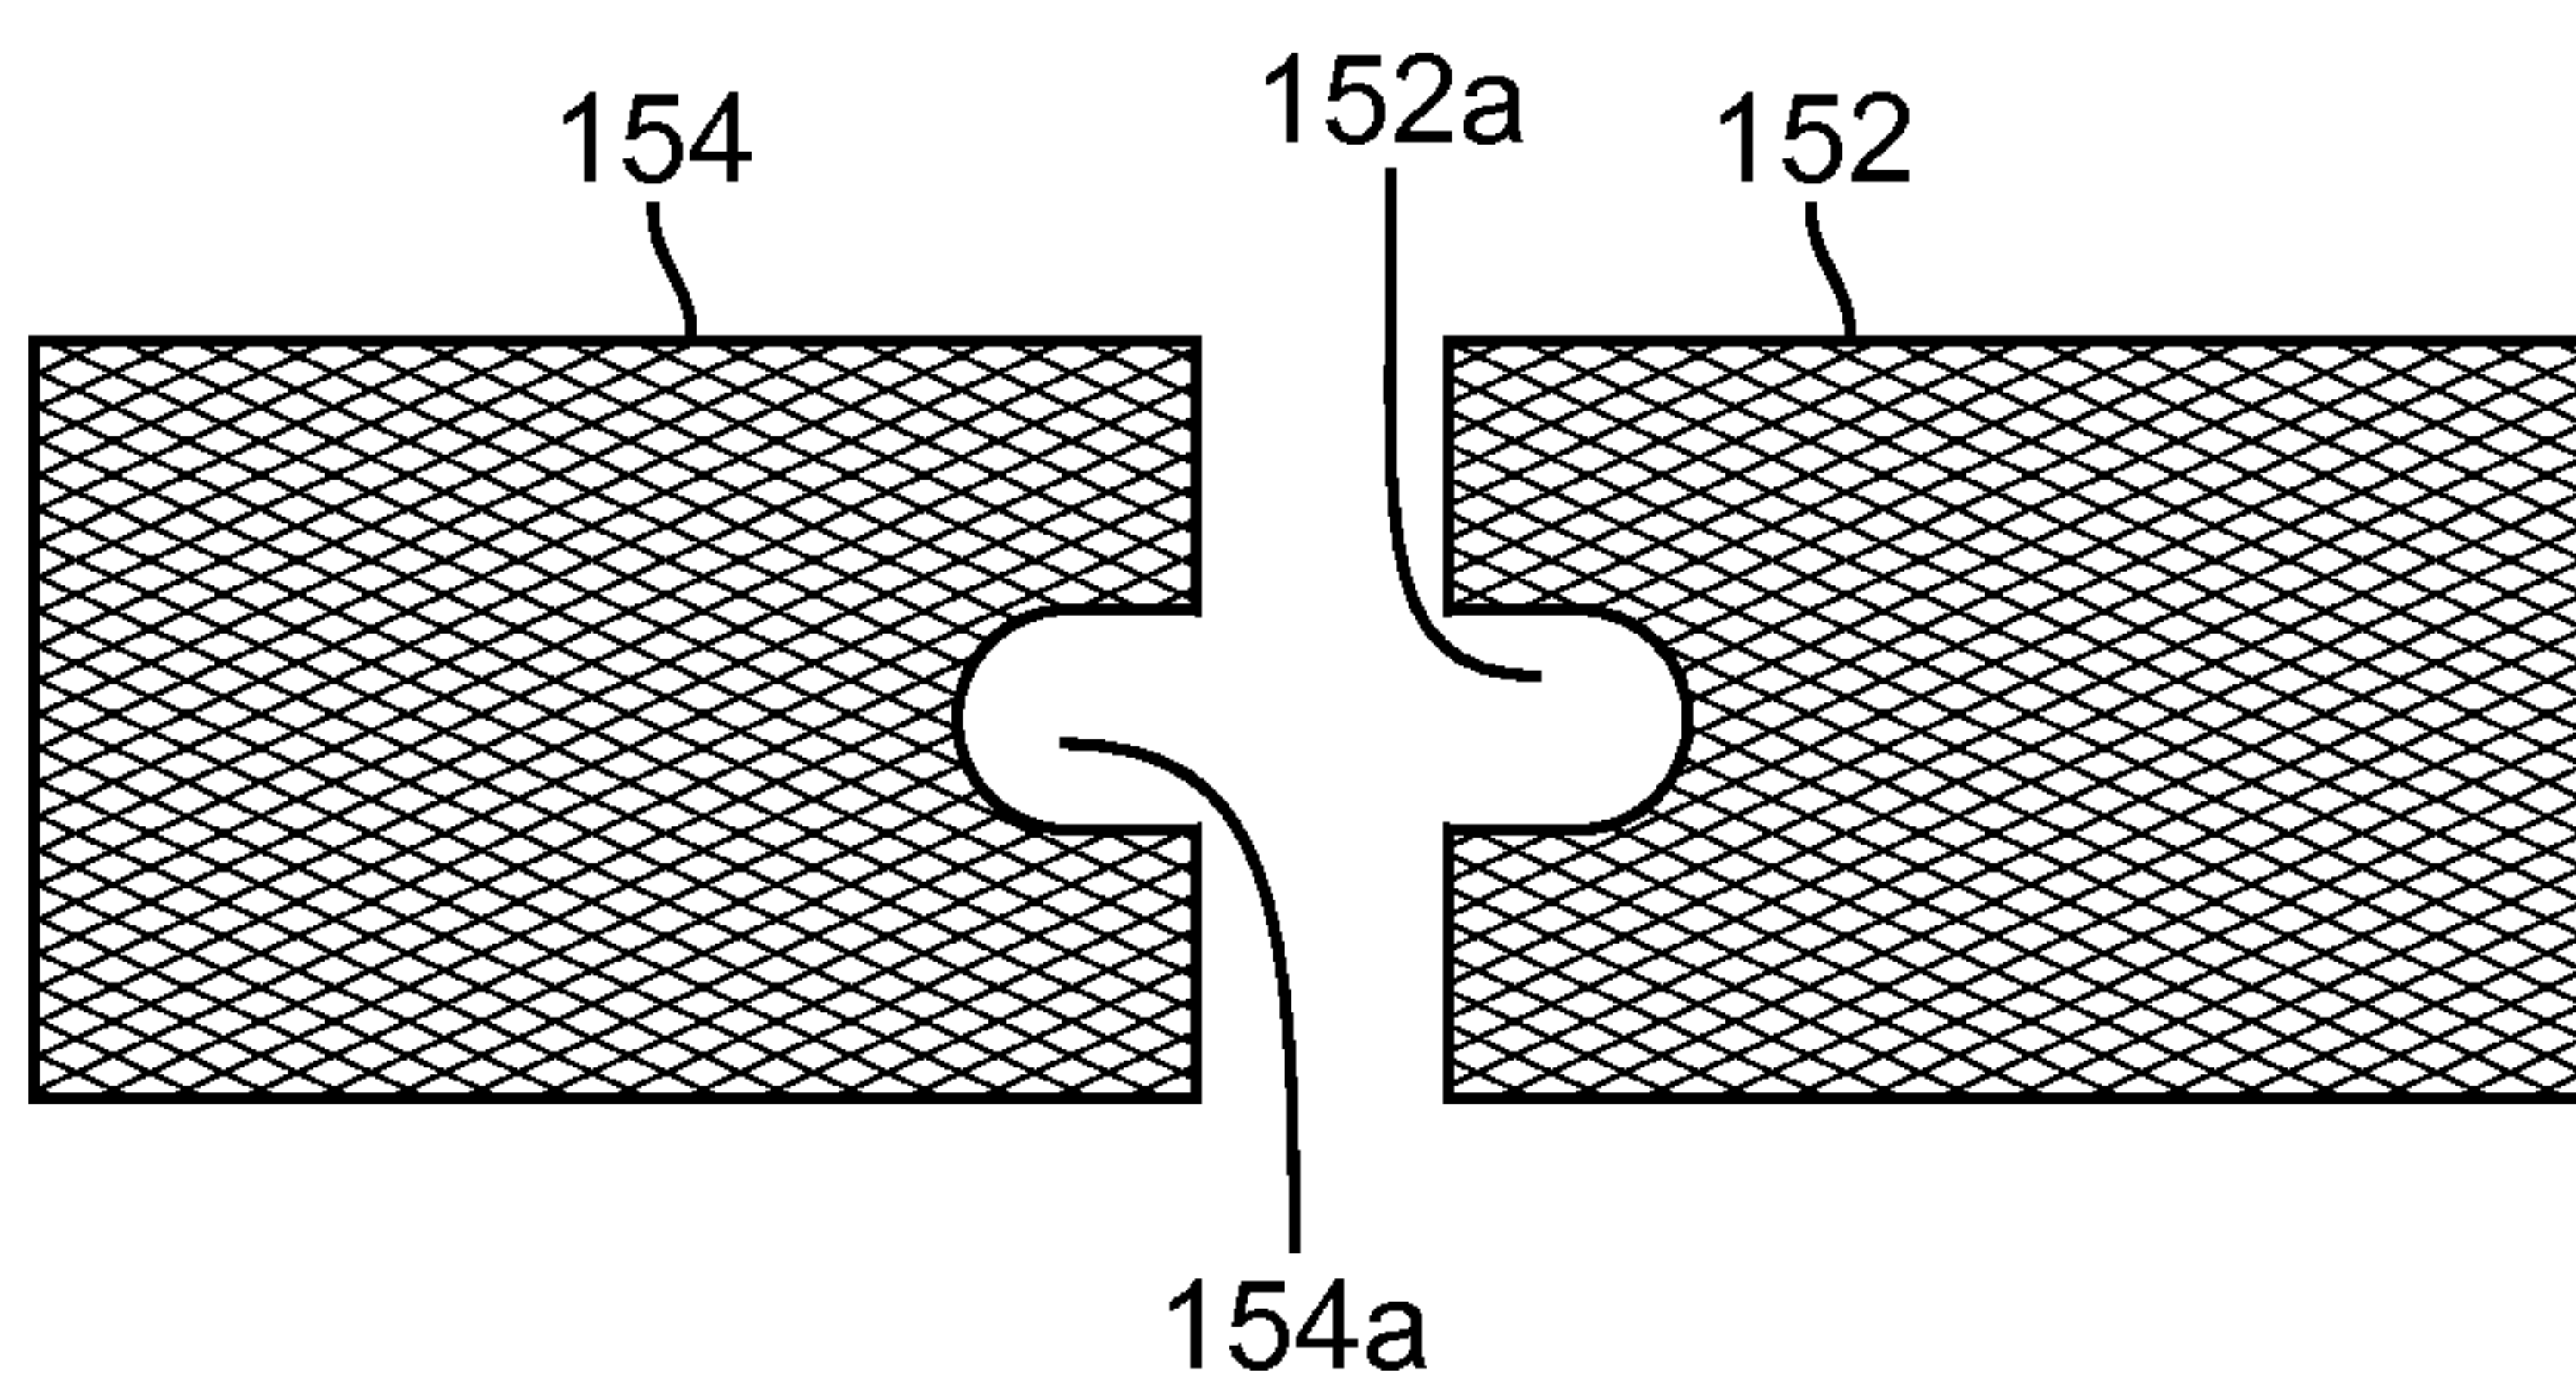


FIG. 3B

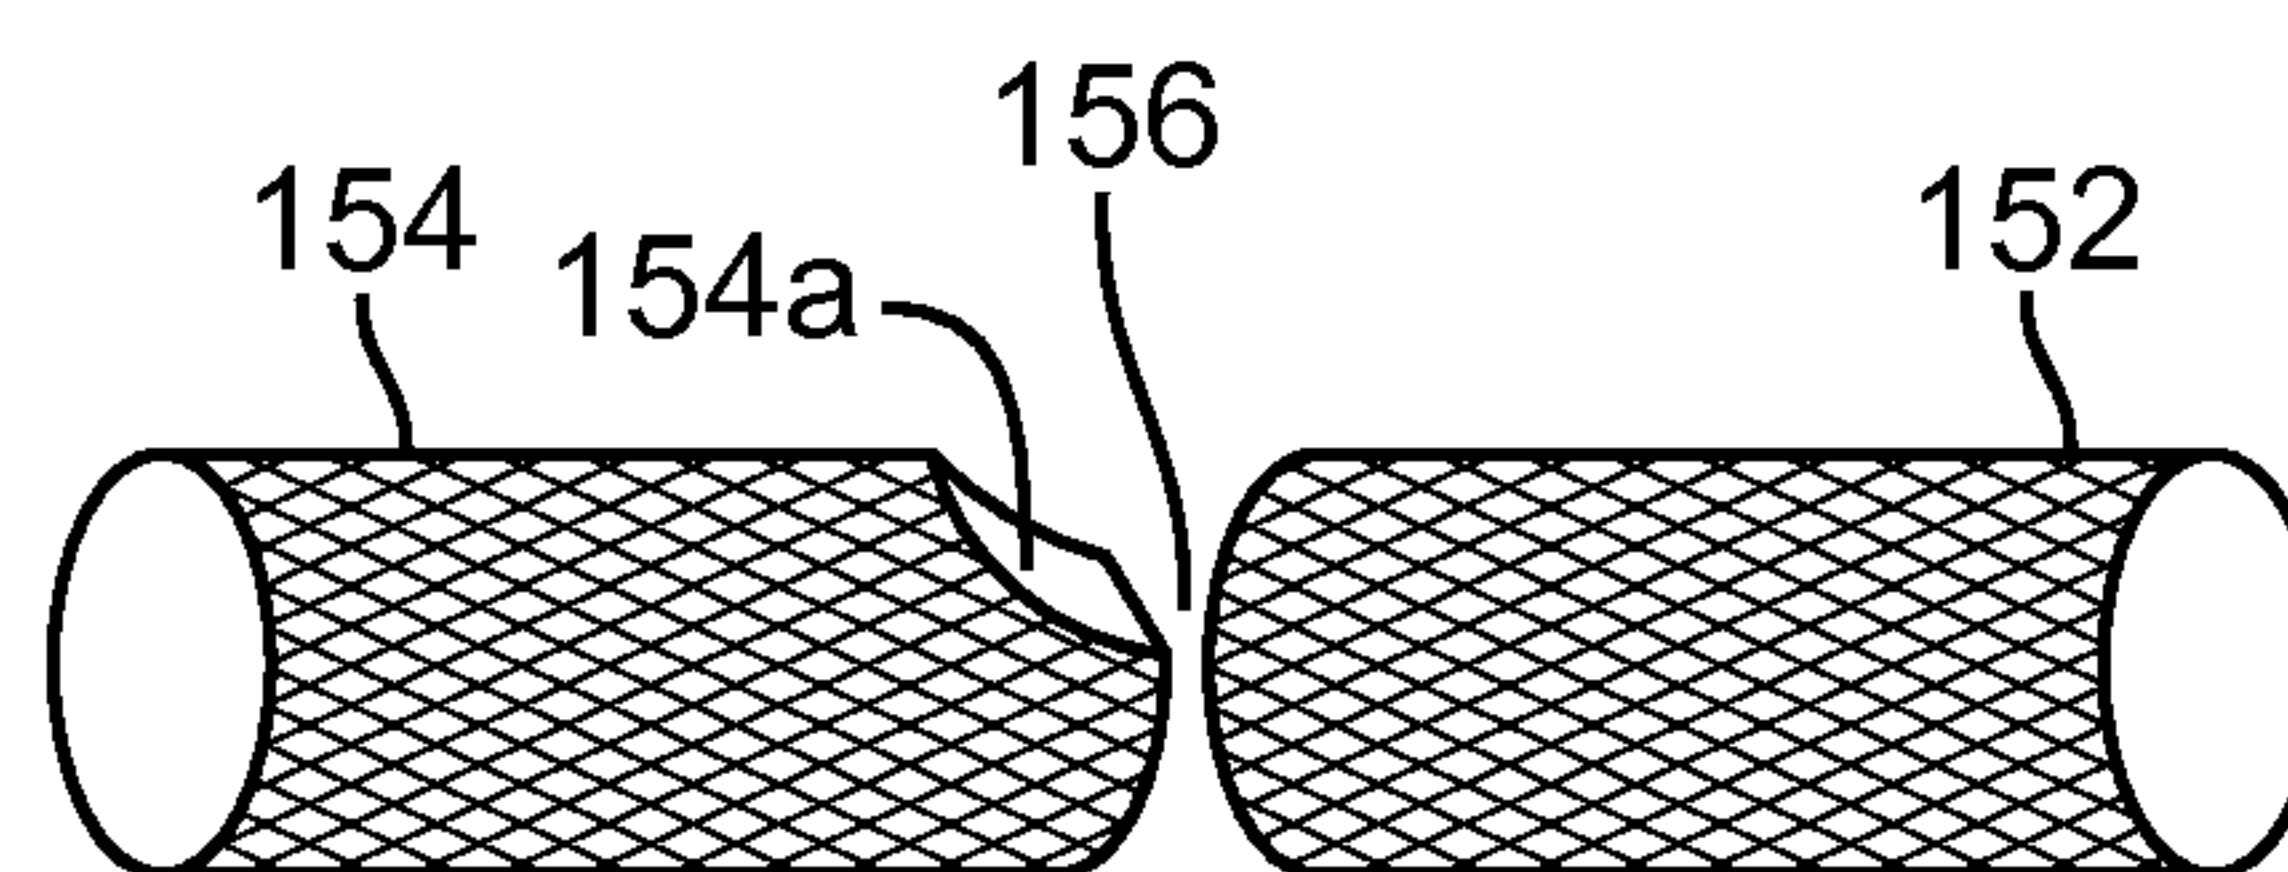


FIG. 3C

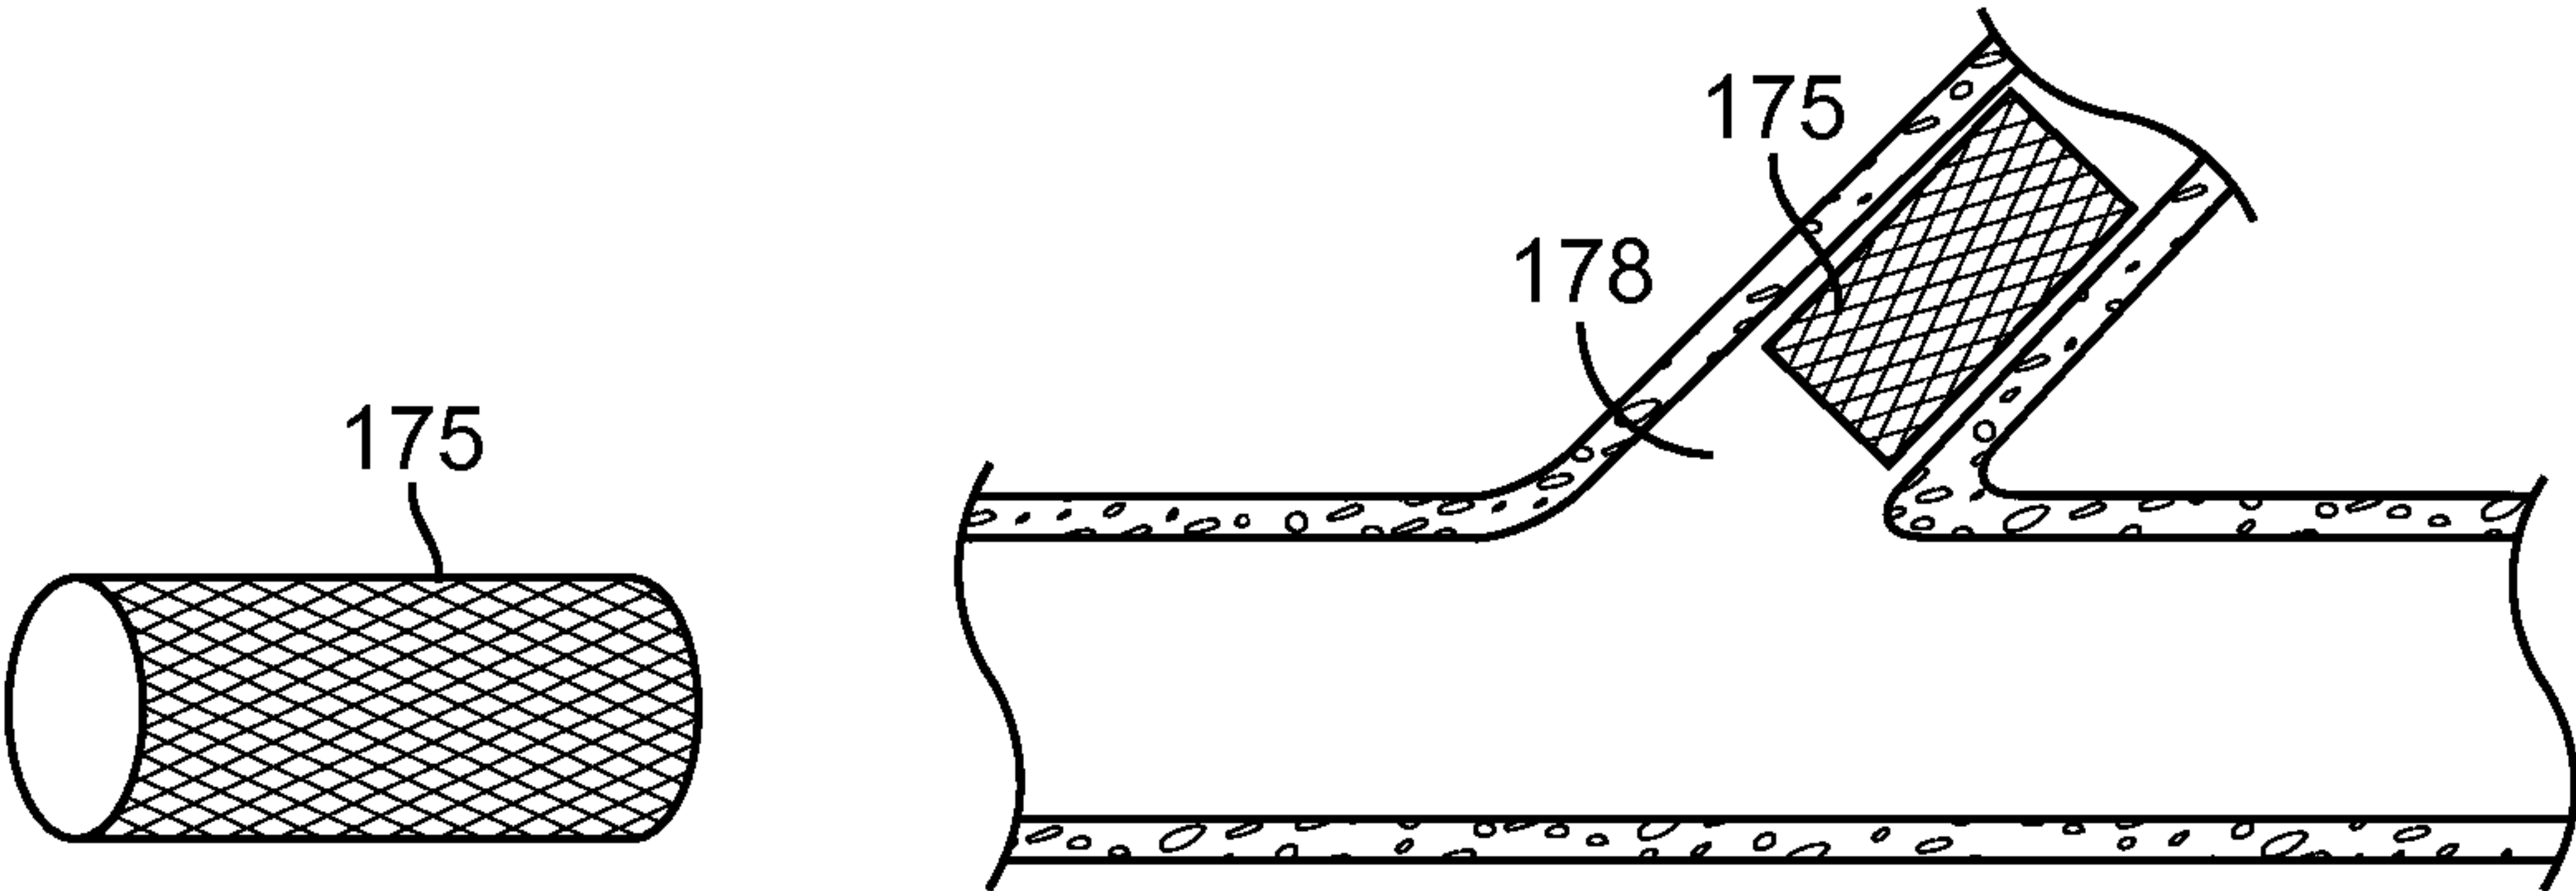


FIG. 3D

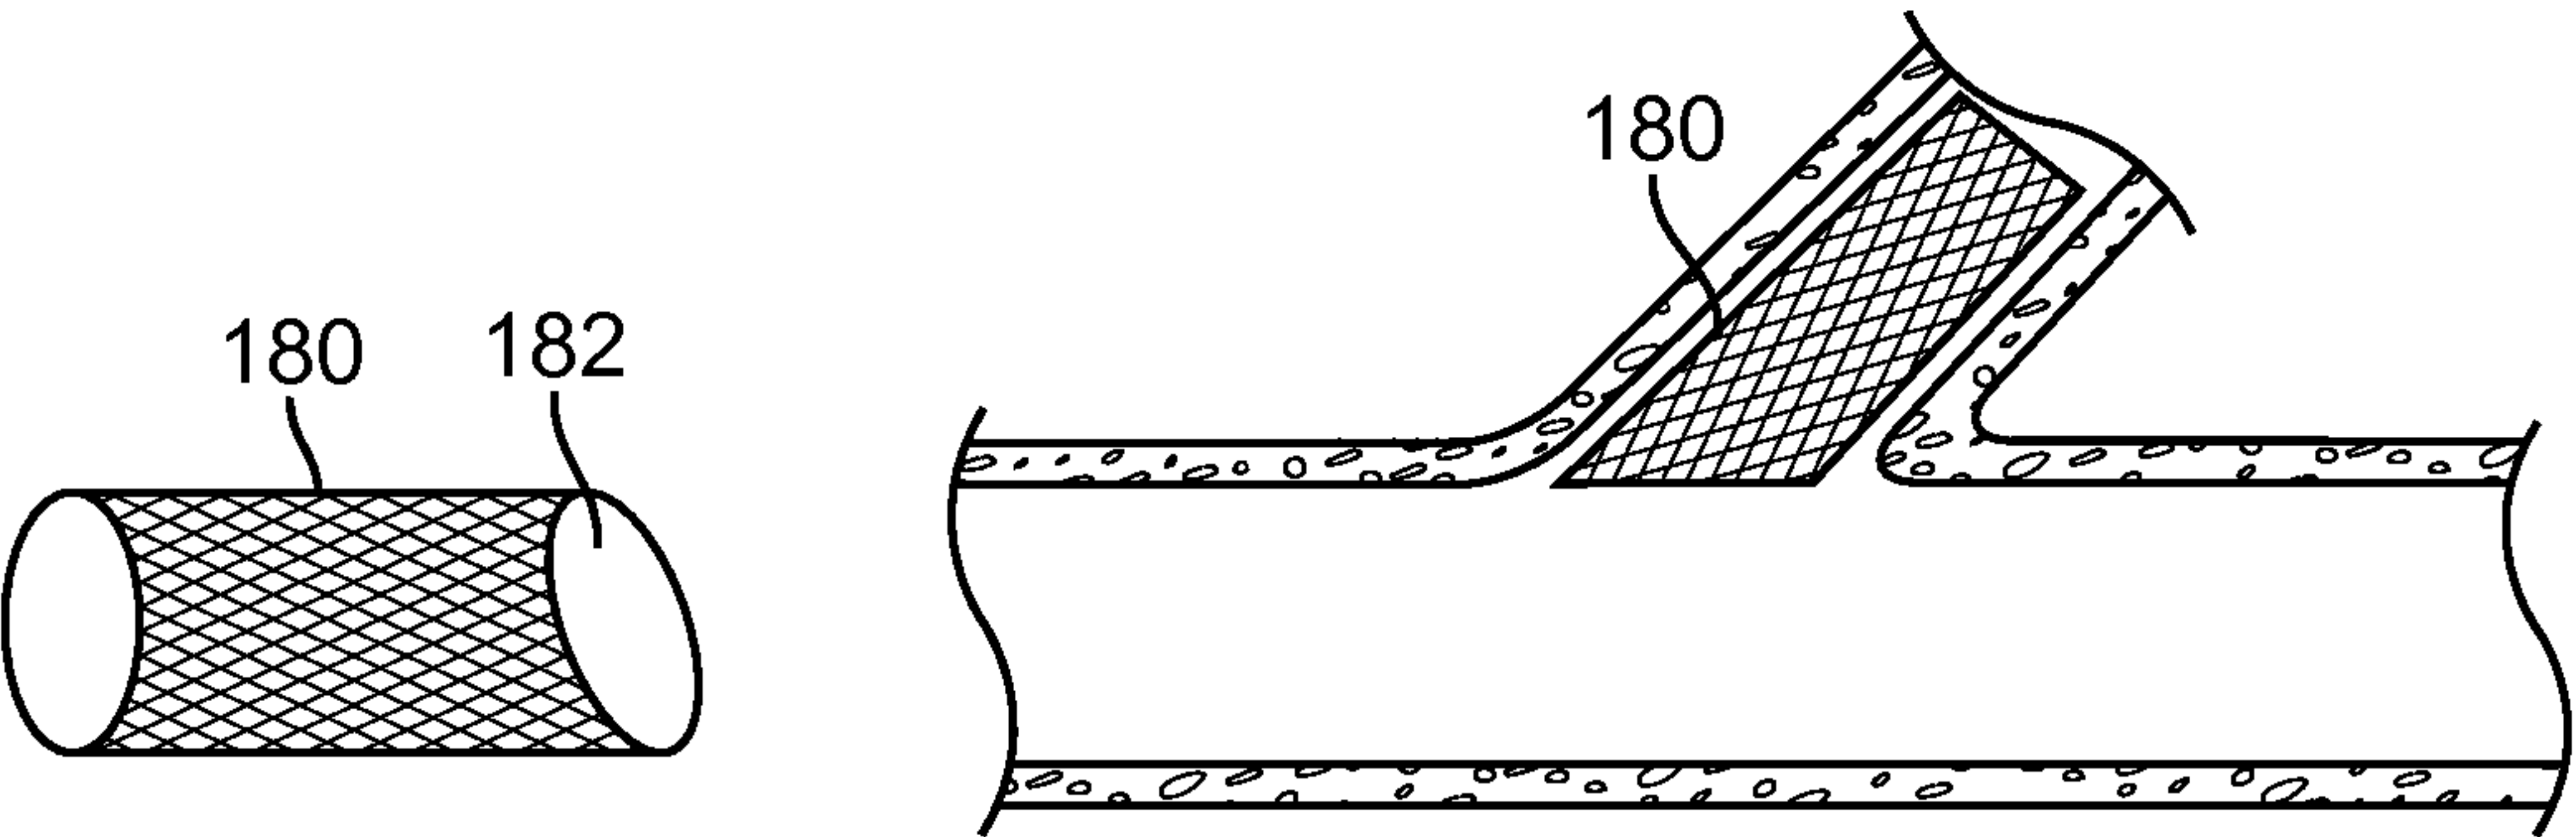


FIG. 3E

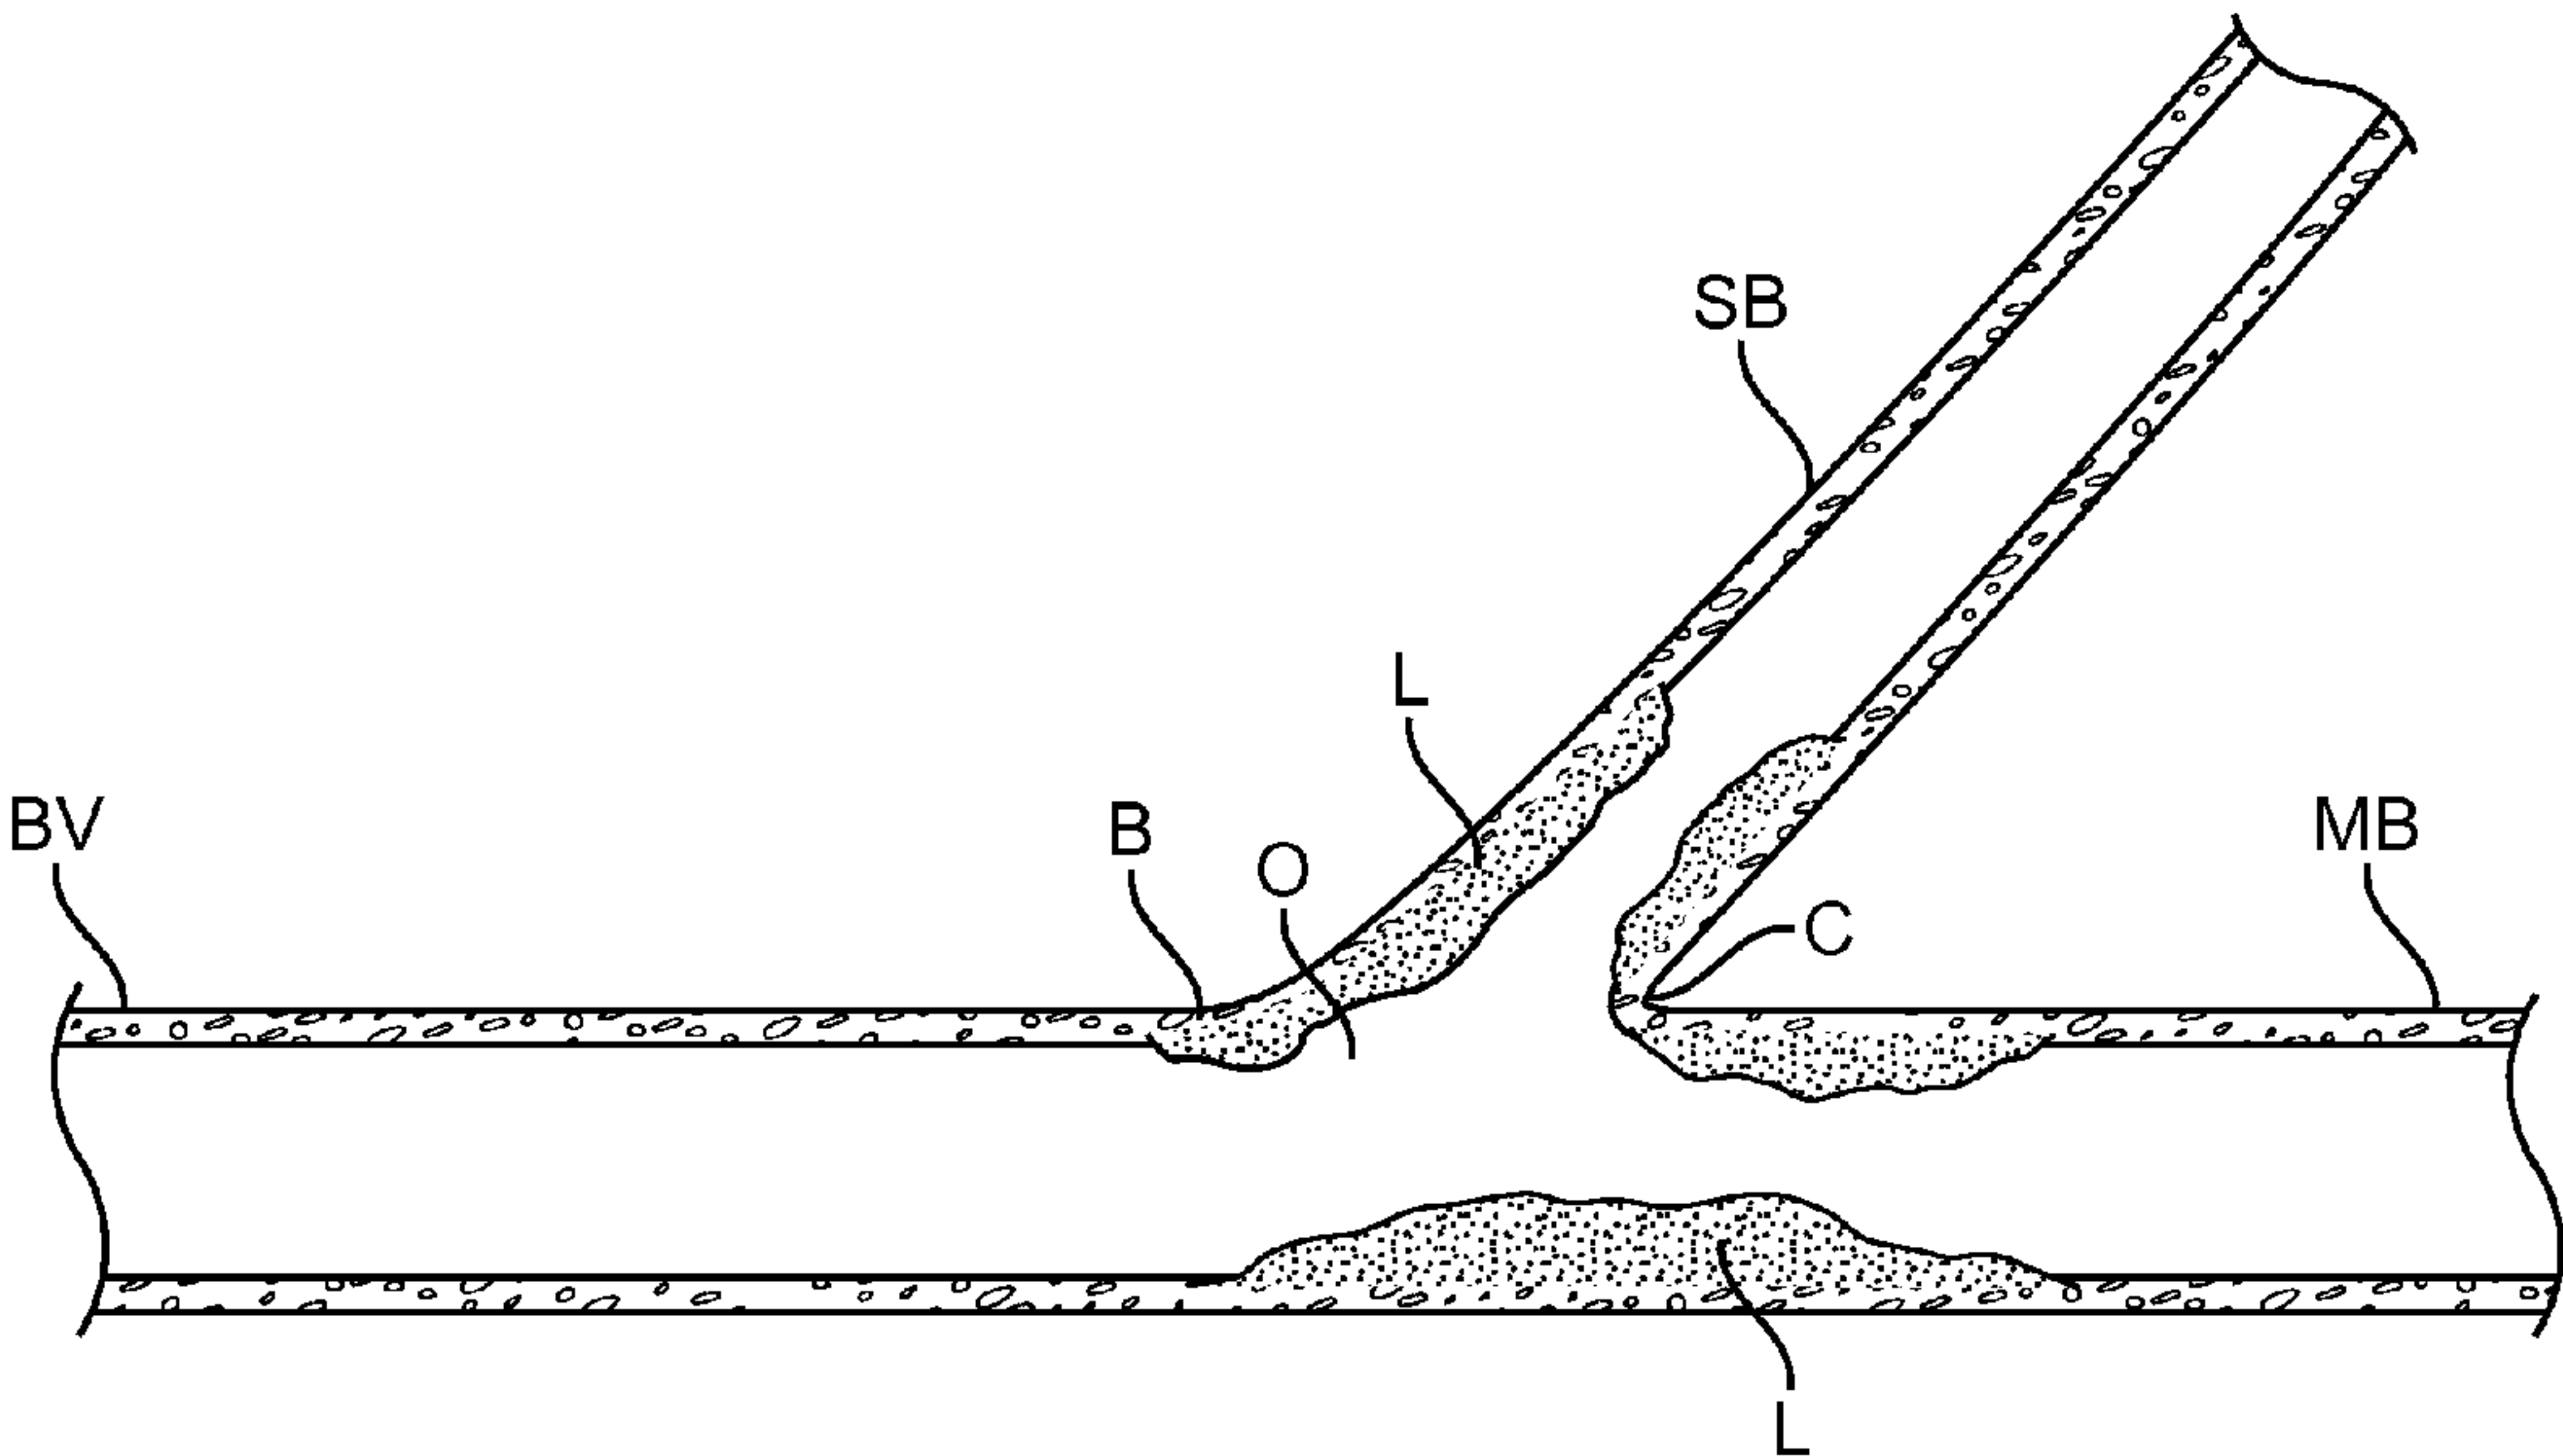


FIG. 4A

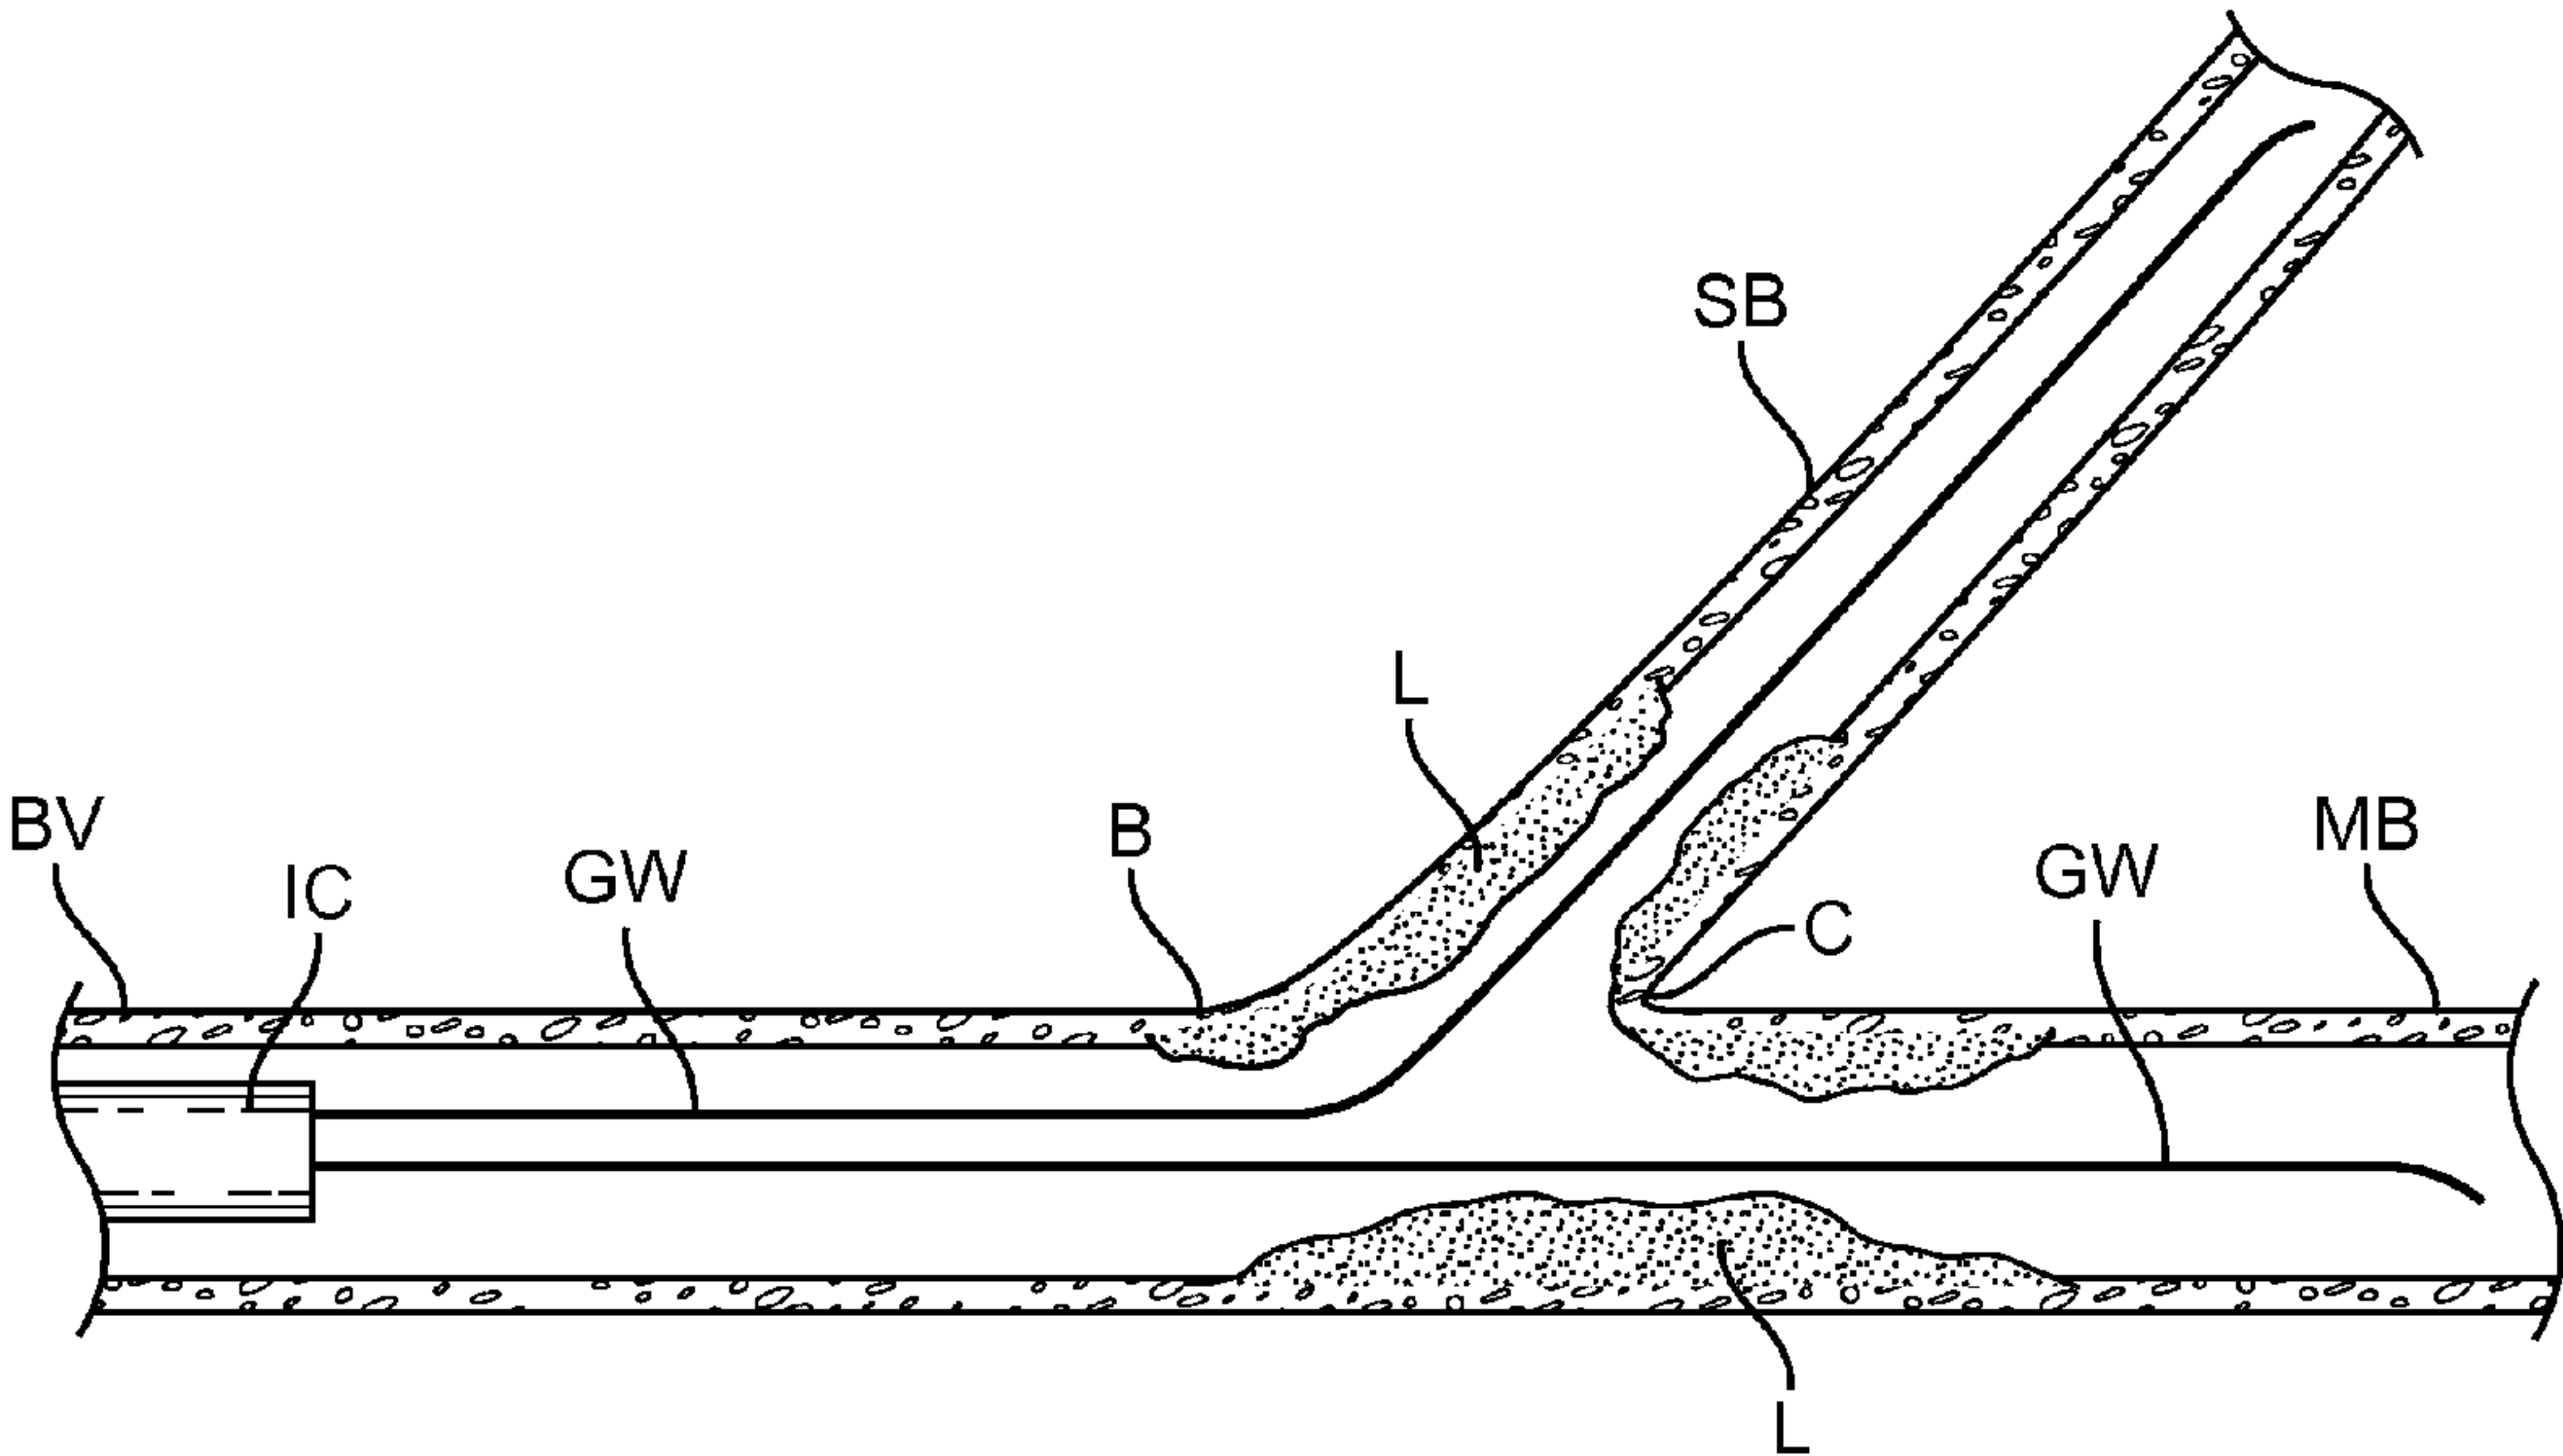


FIG. 4B

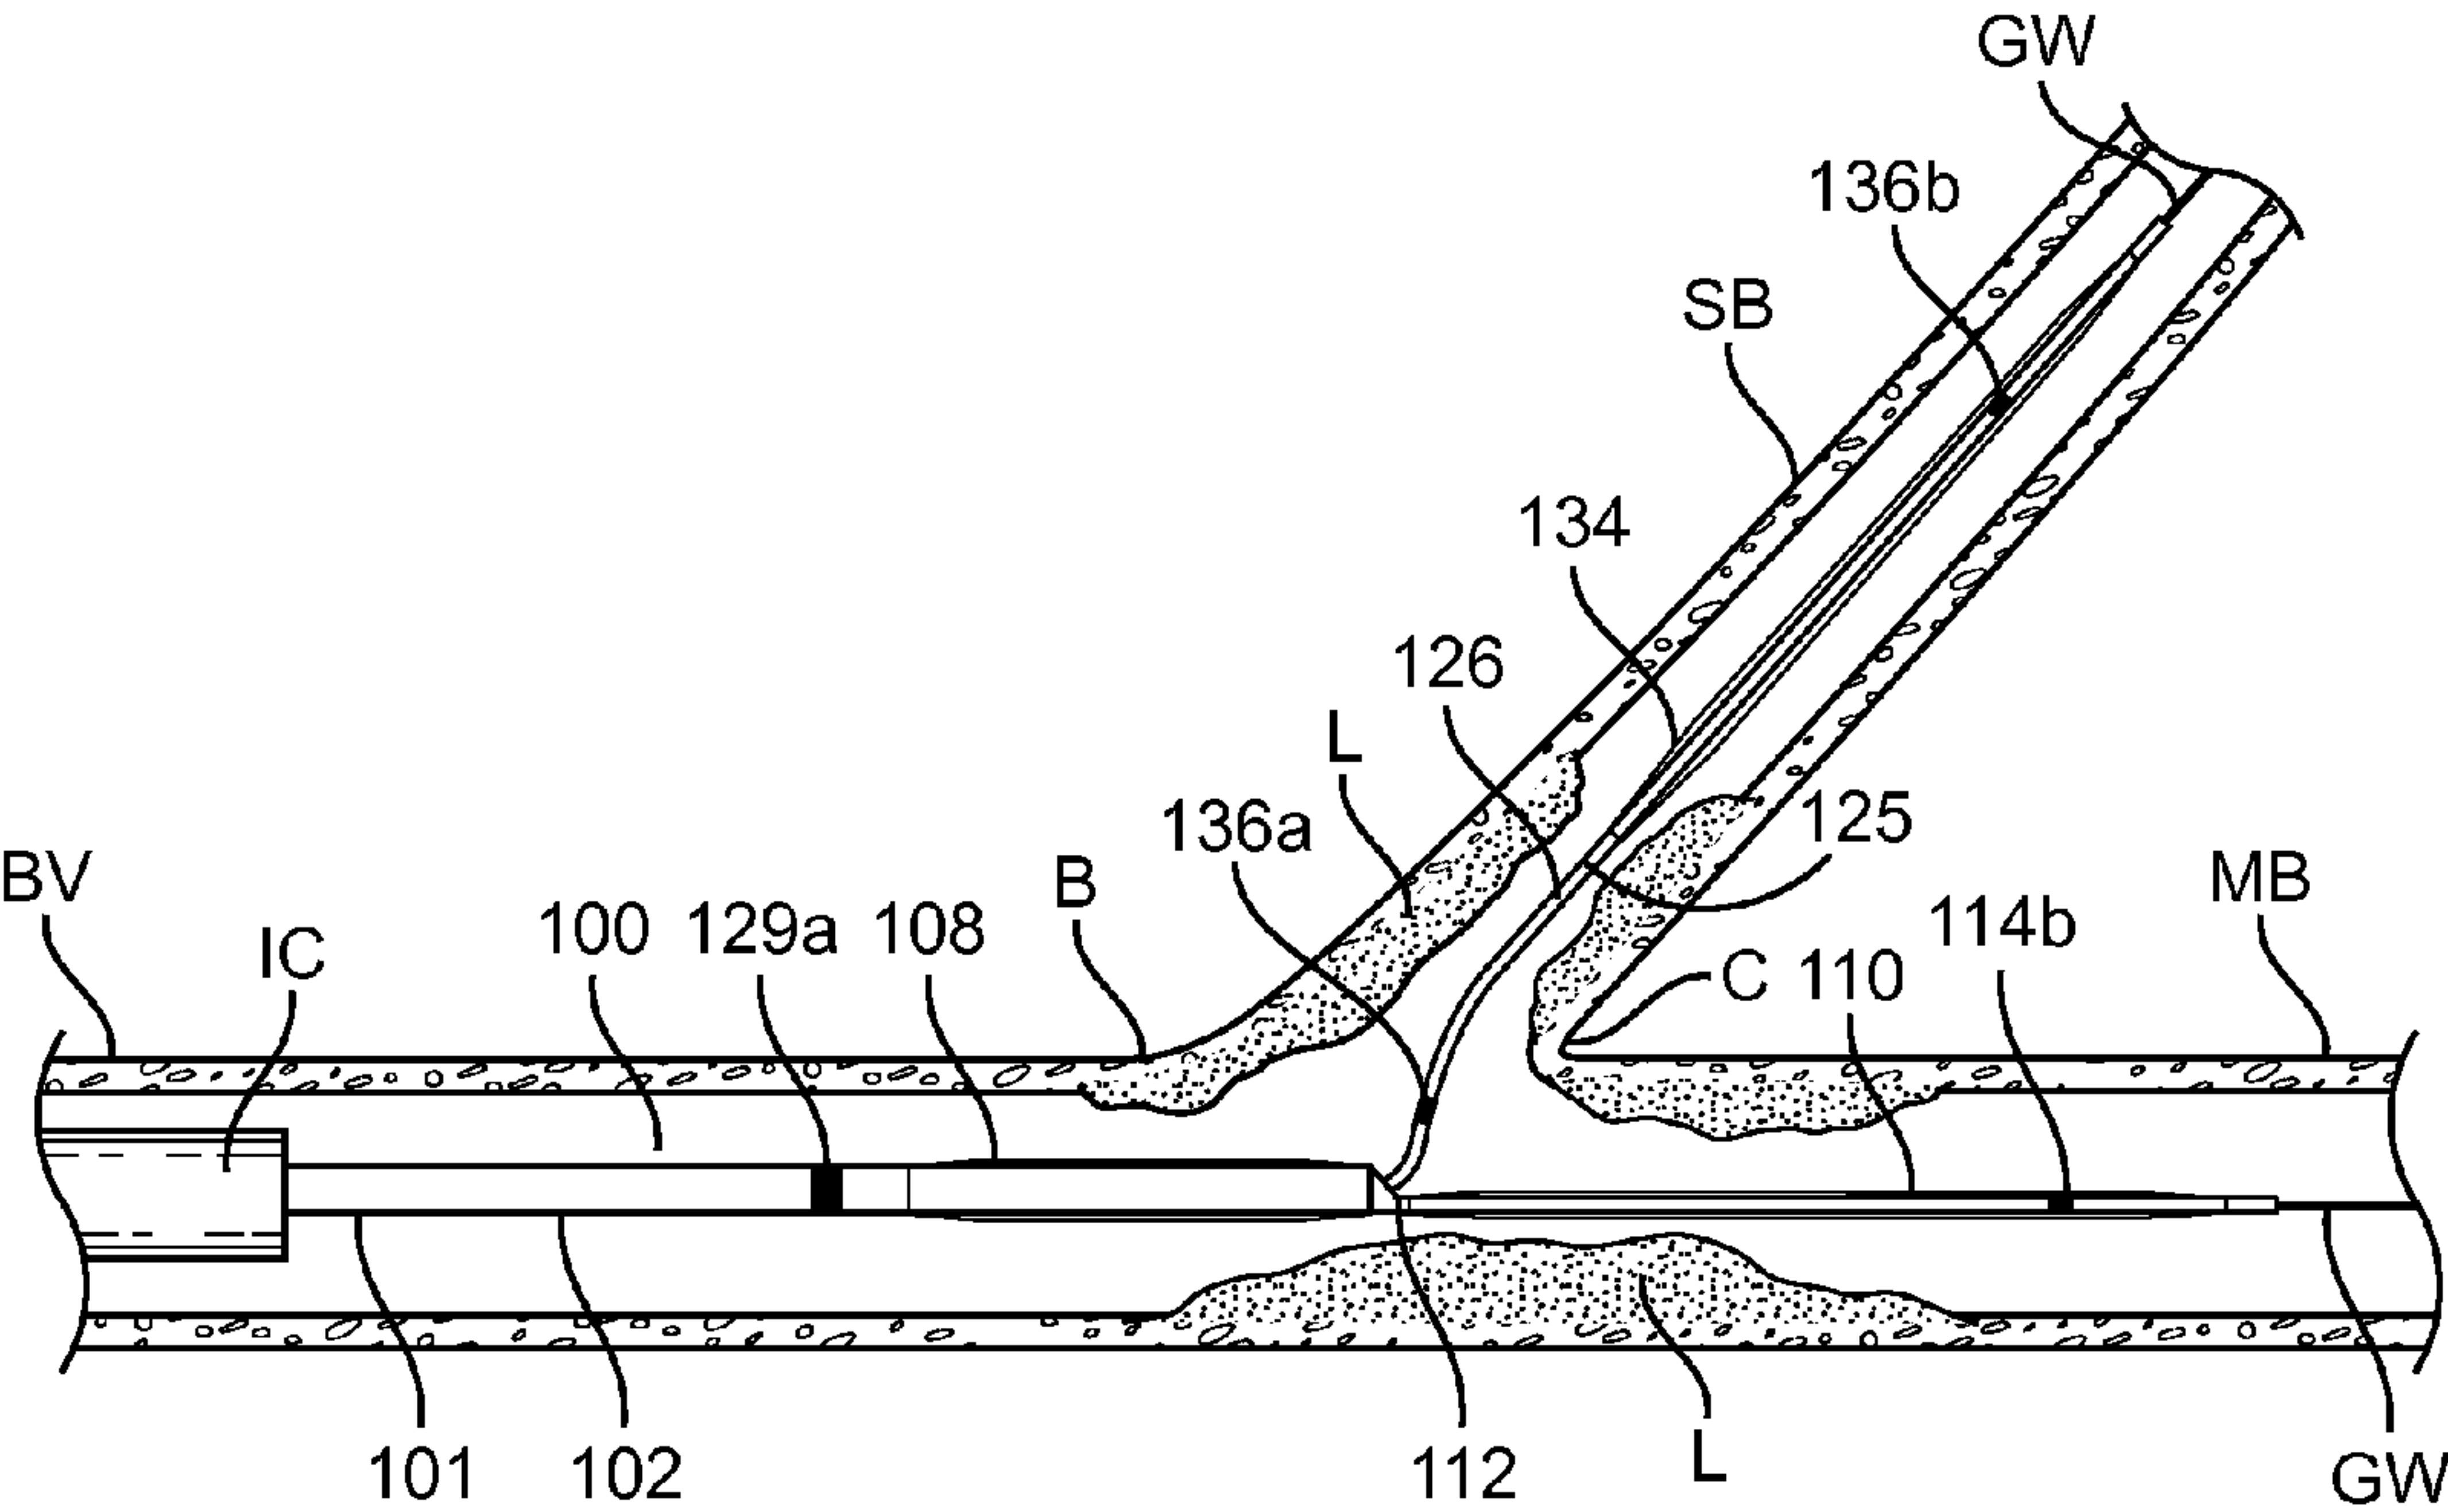


FIG. 4C

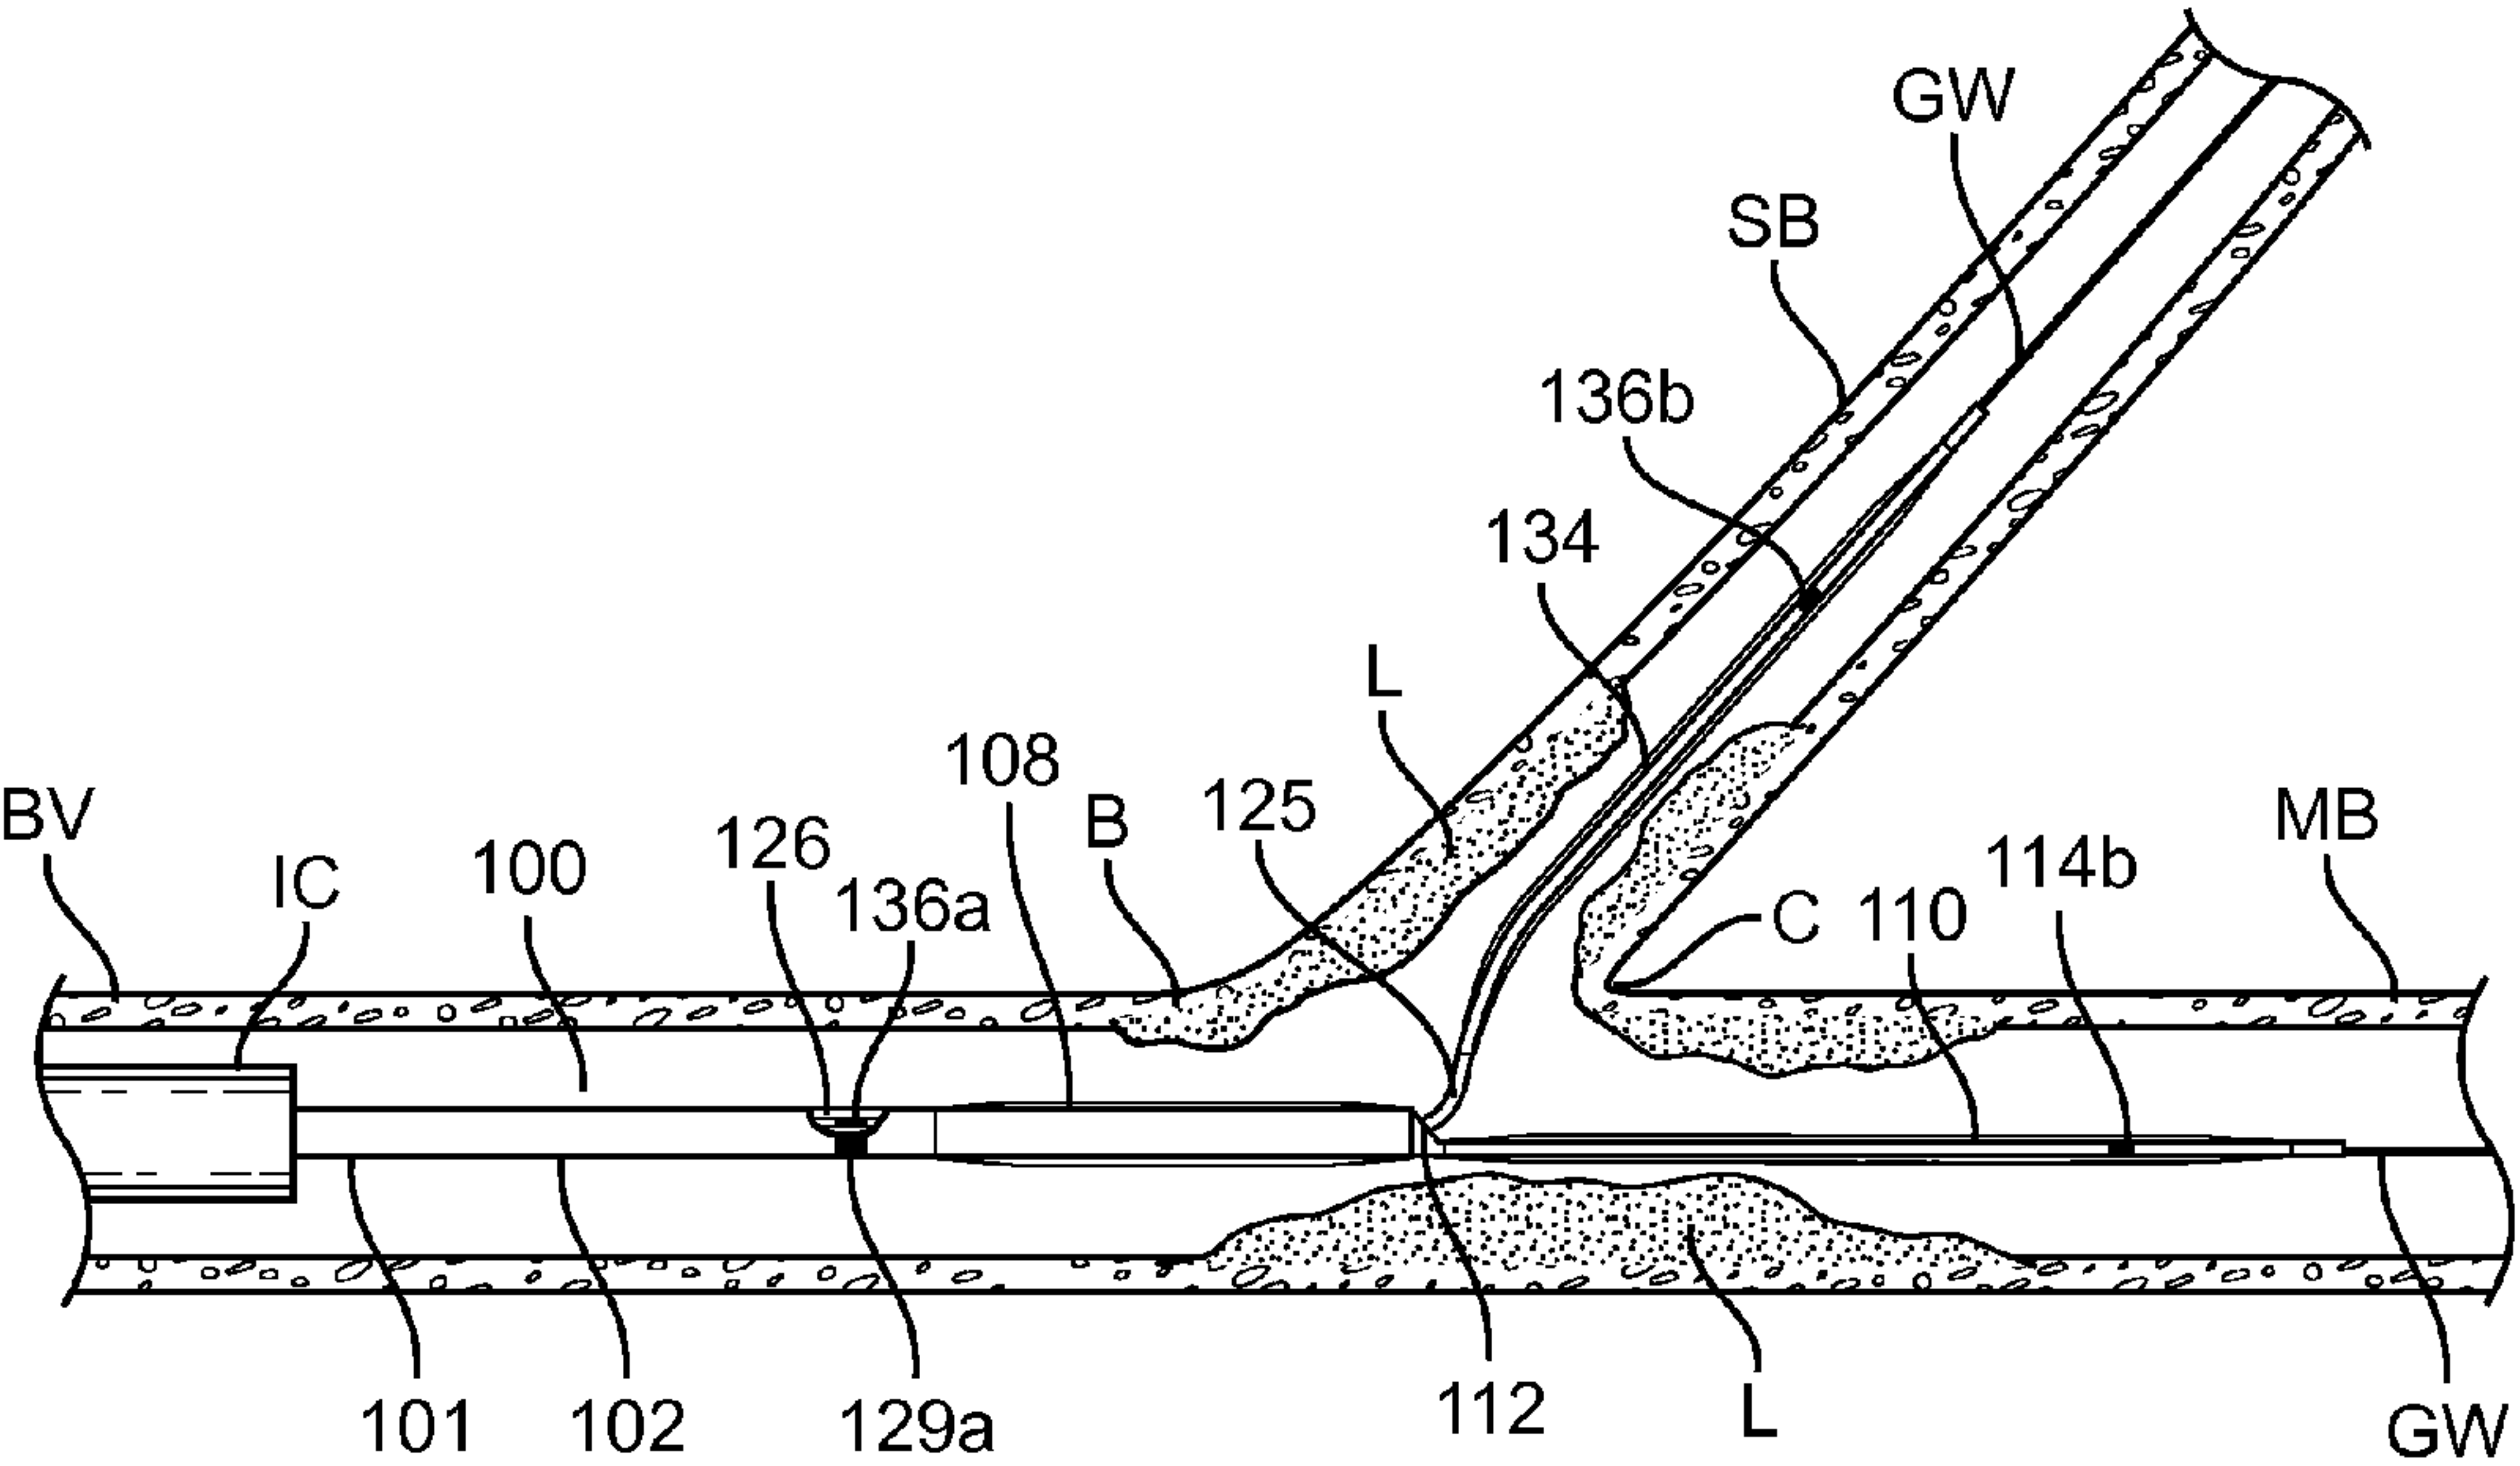


FIG. 4D

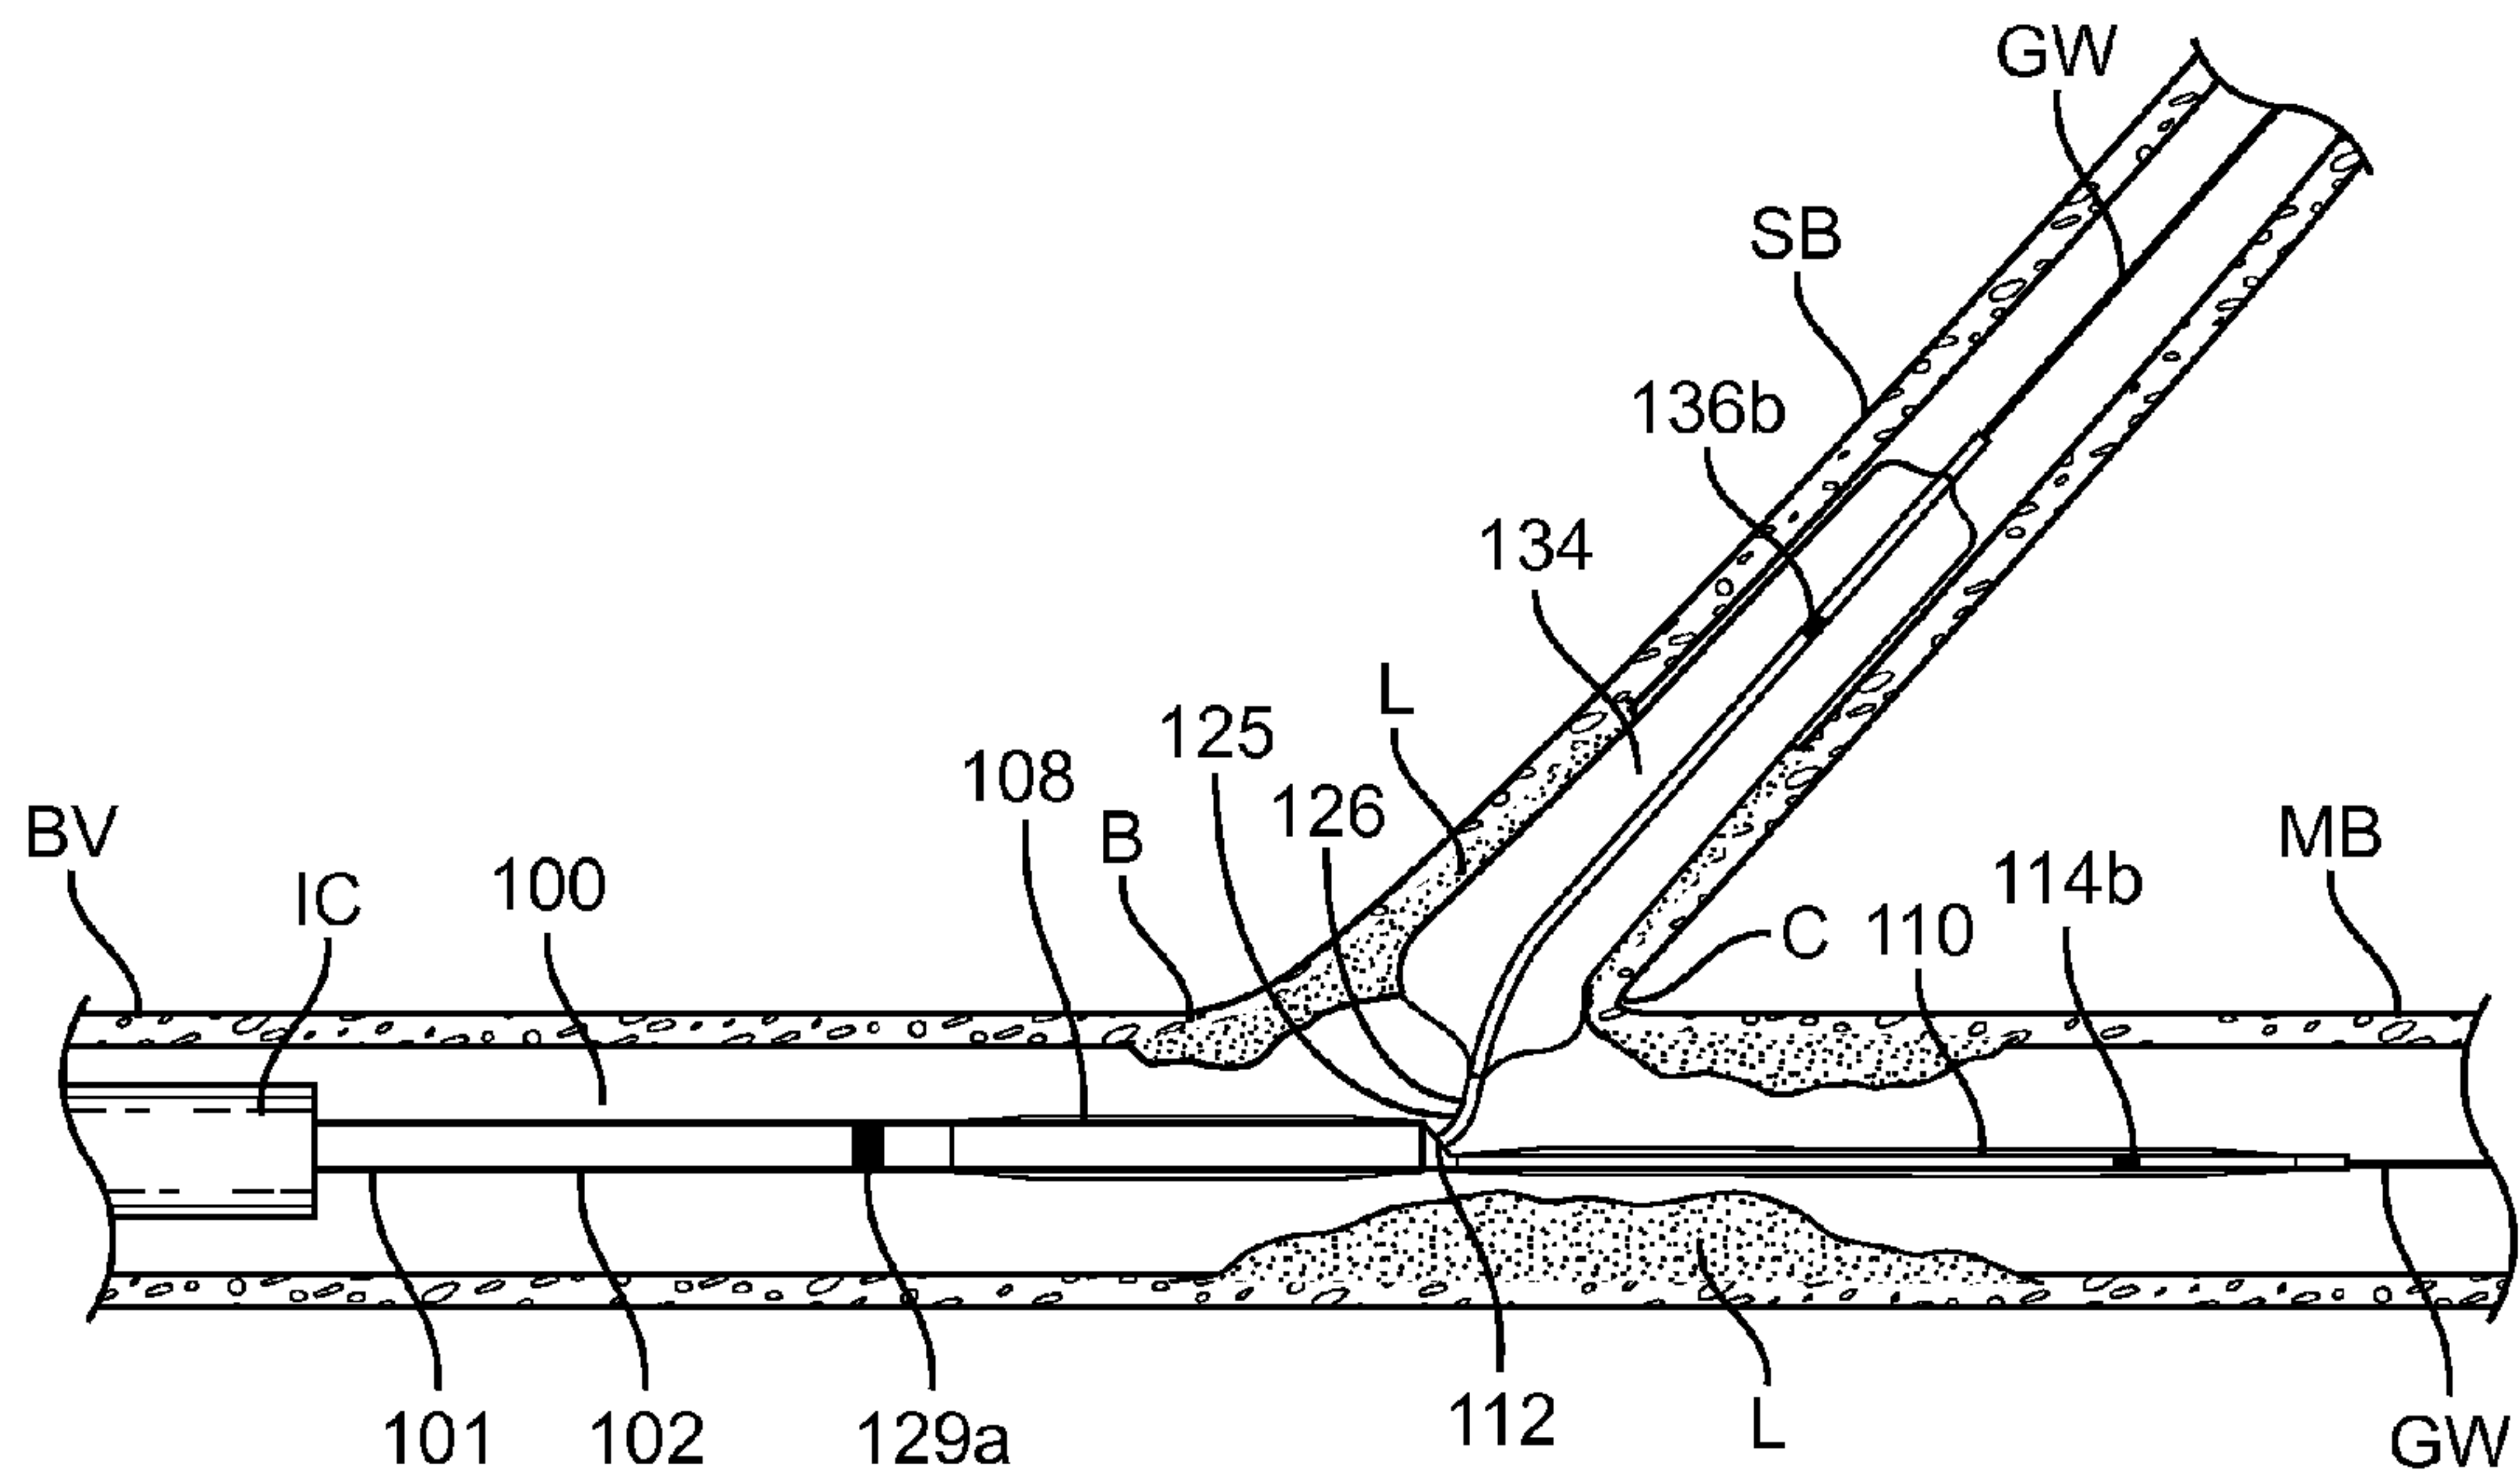


FIG. 4E

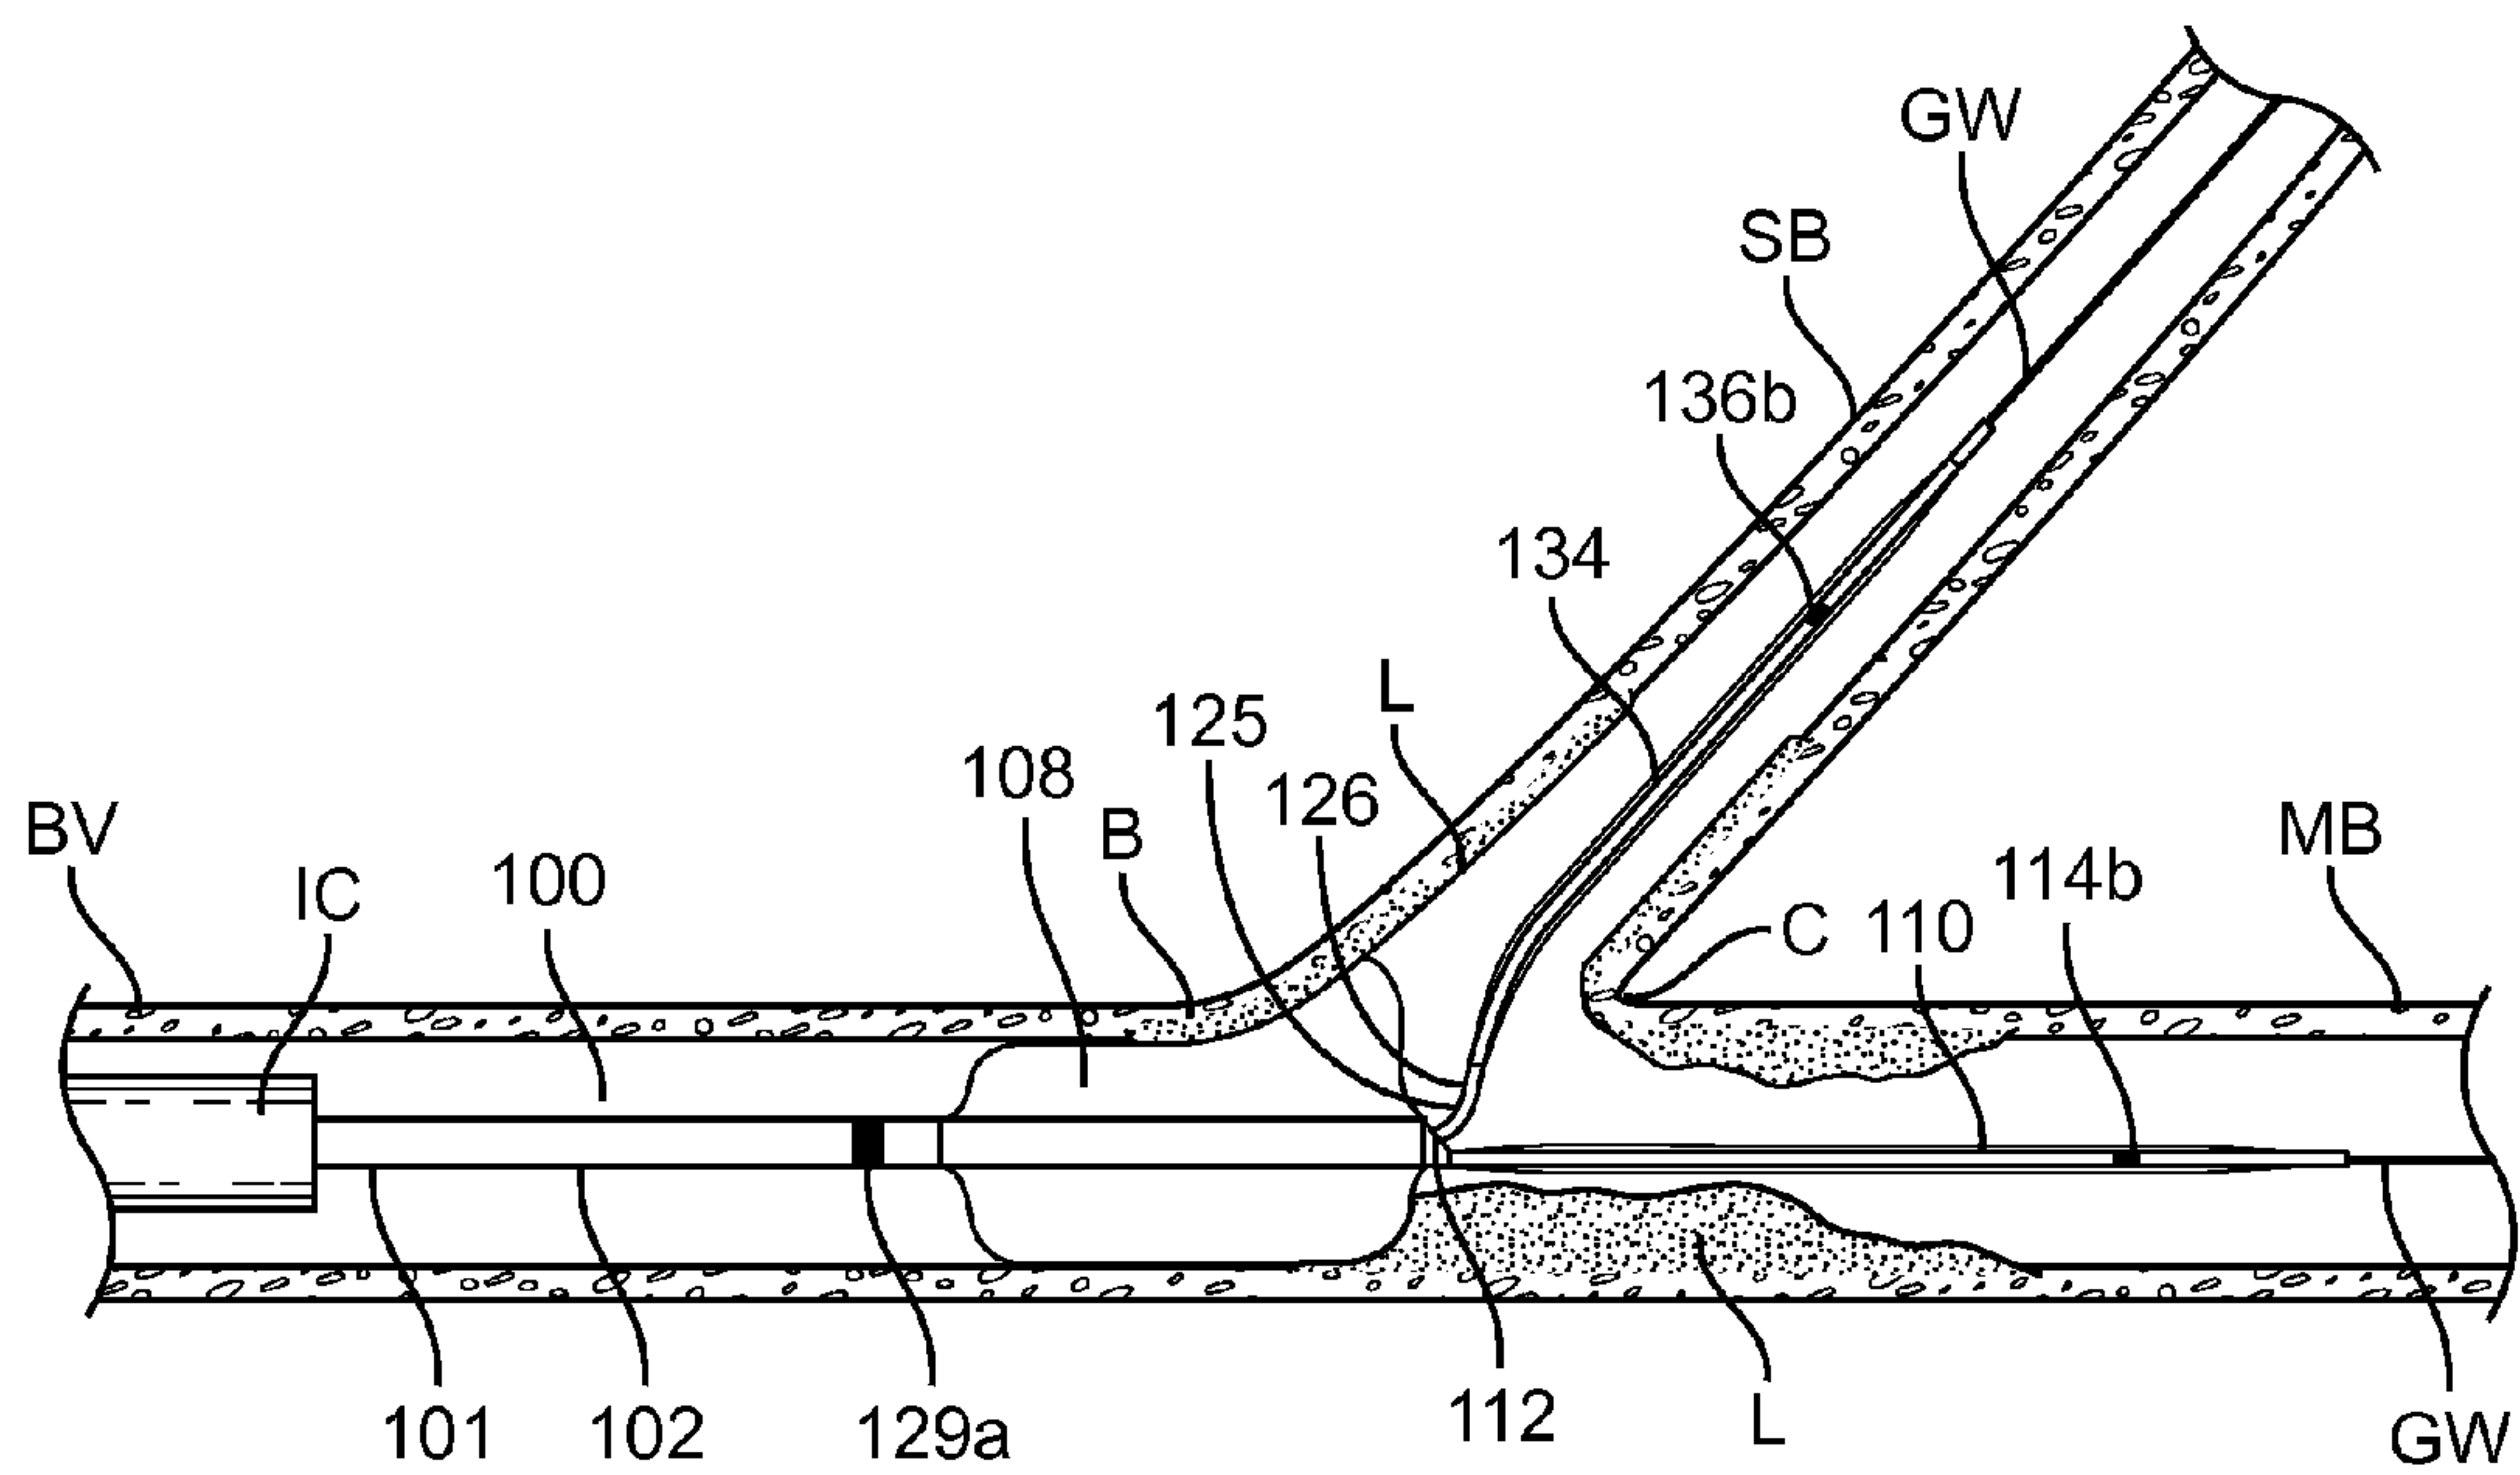


FIG. 4F

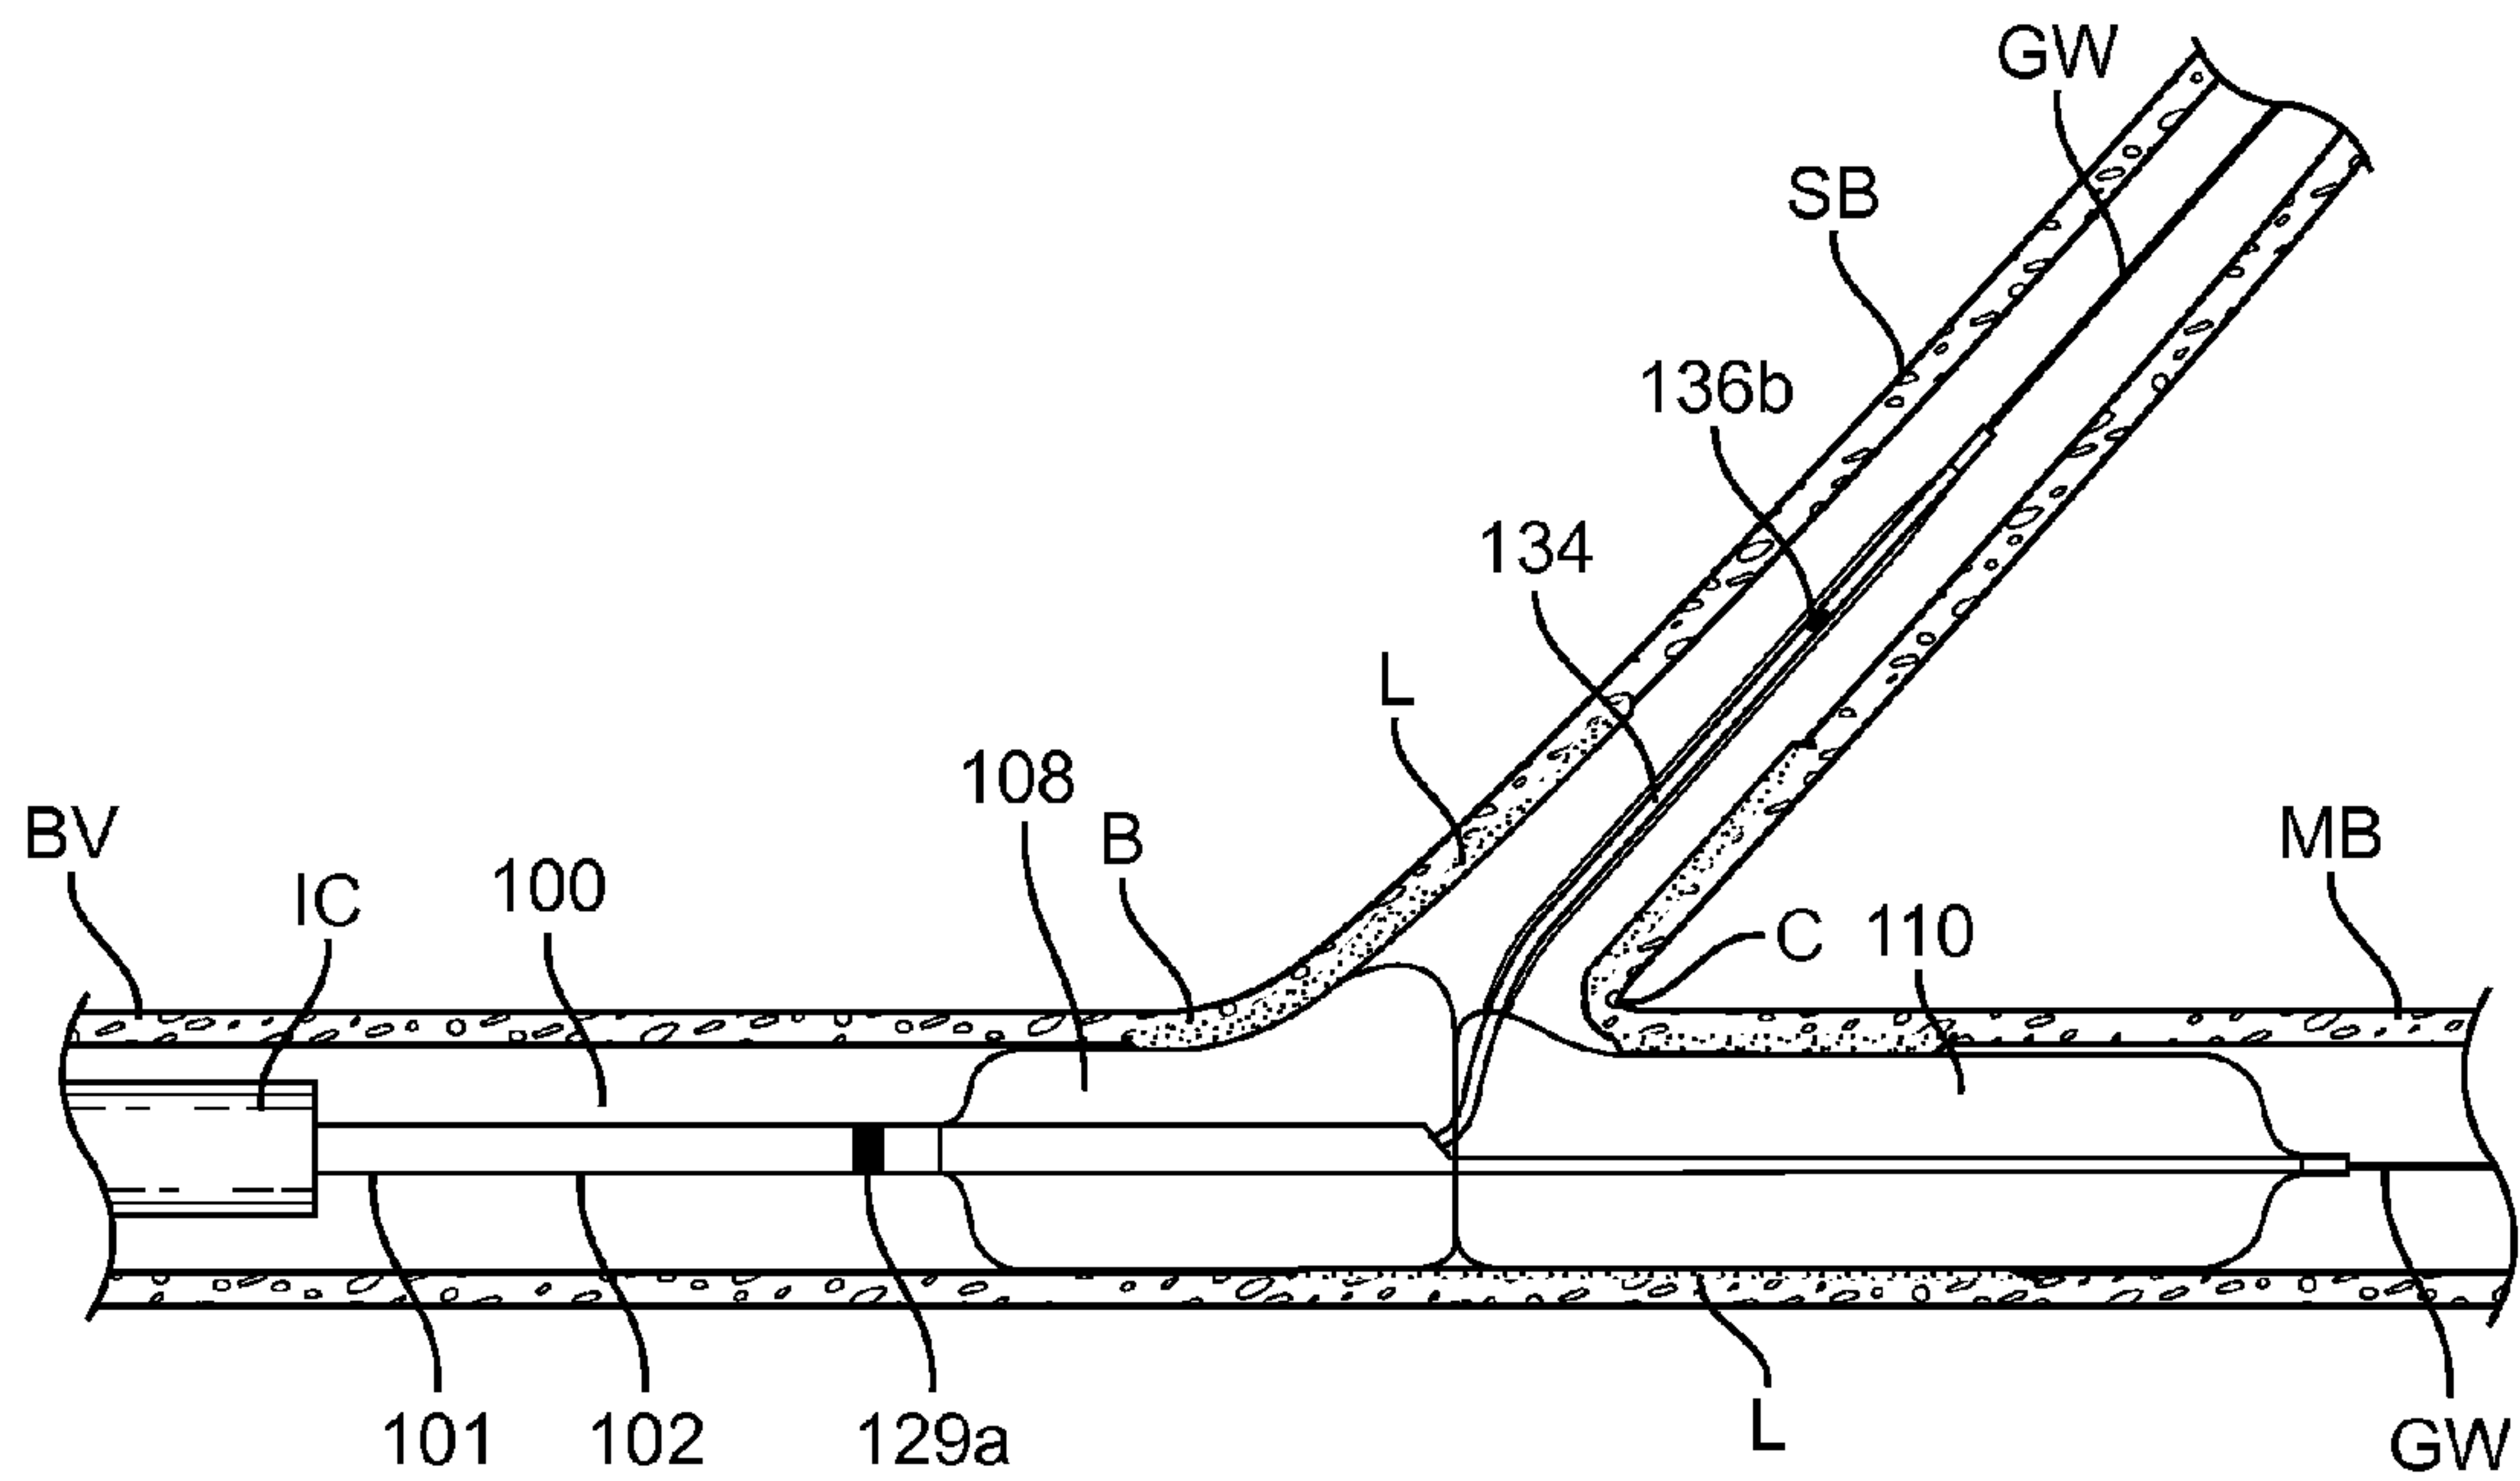


FIG. 4G

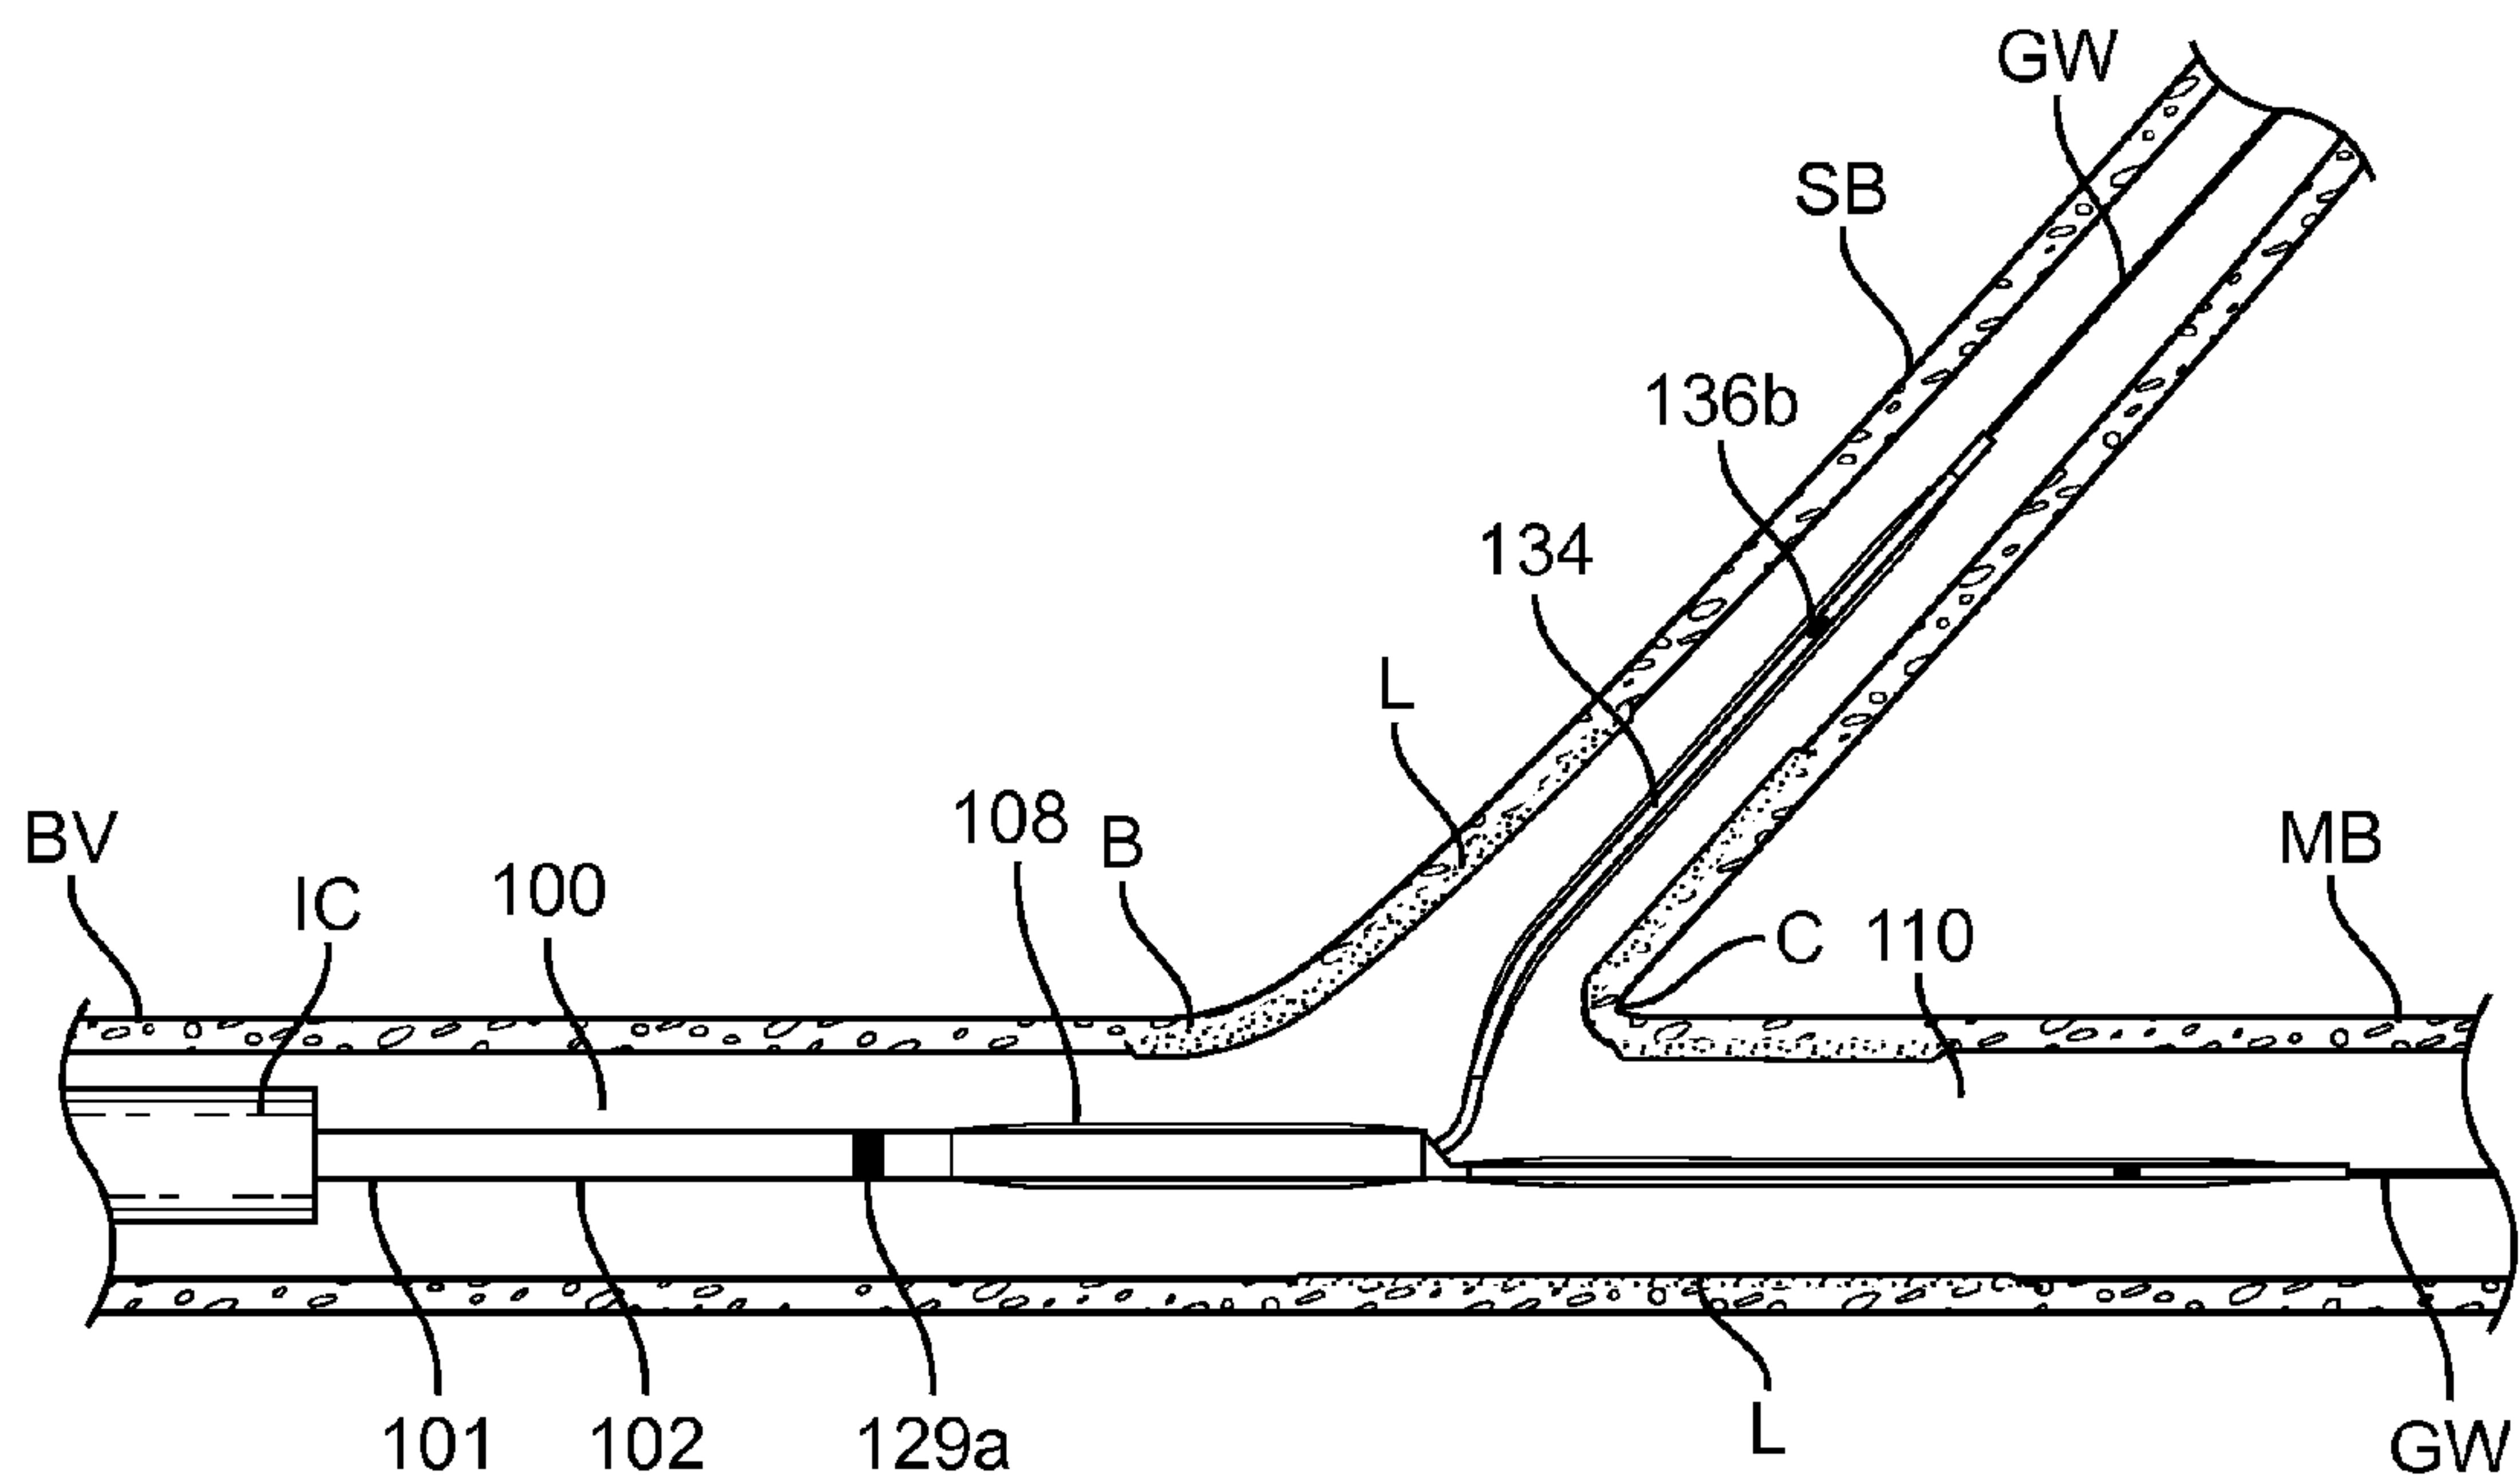


FIG. 4H

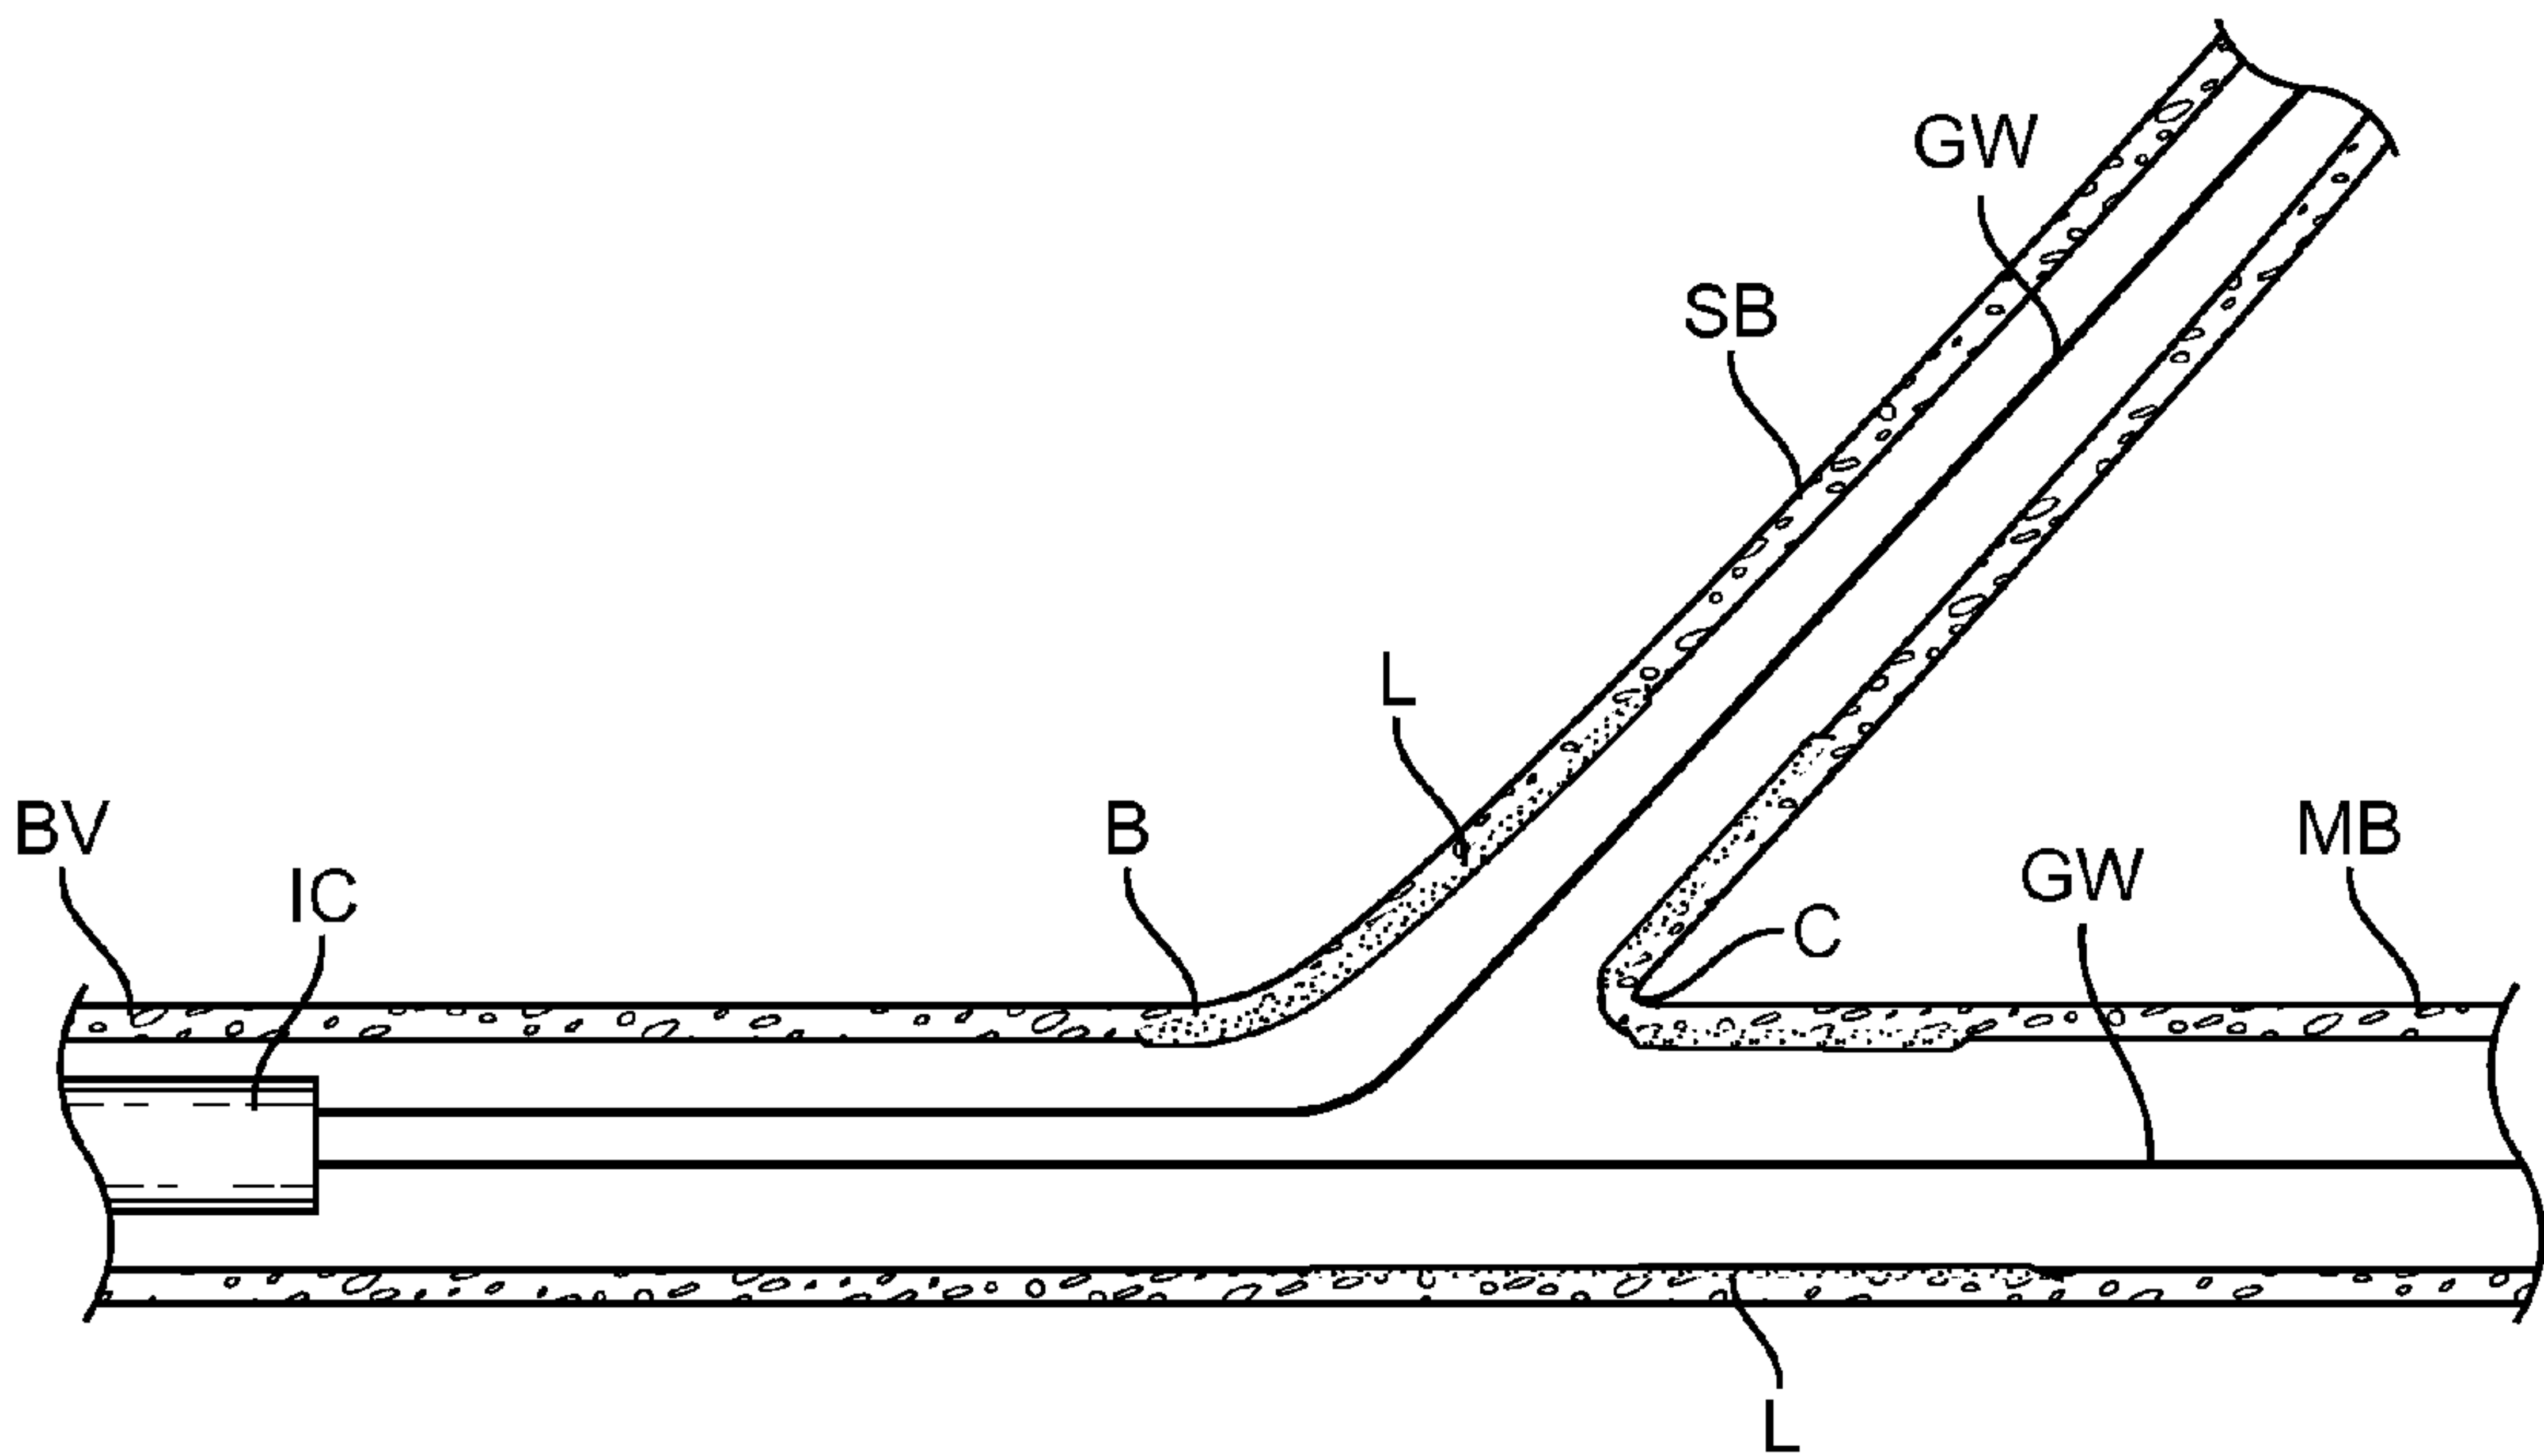


FIG. 4I

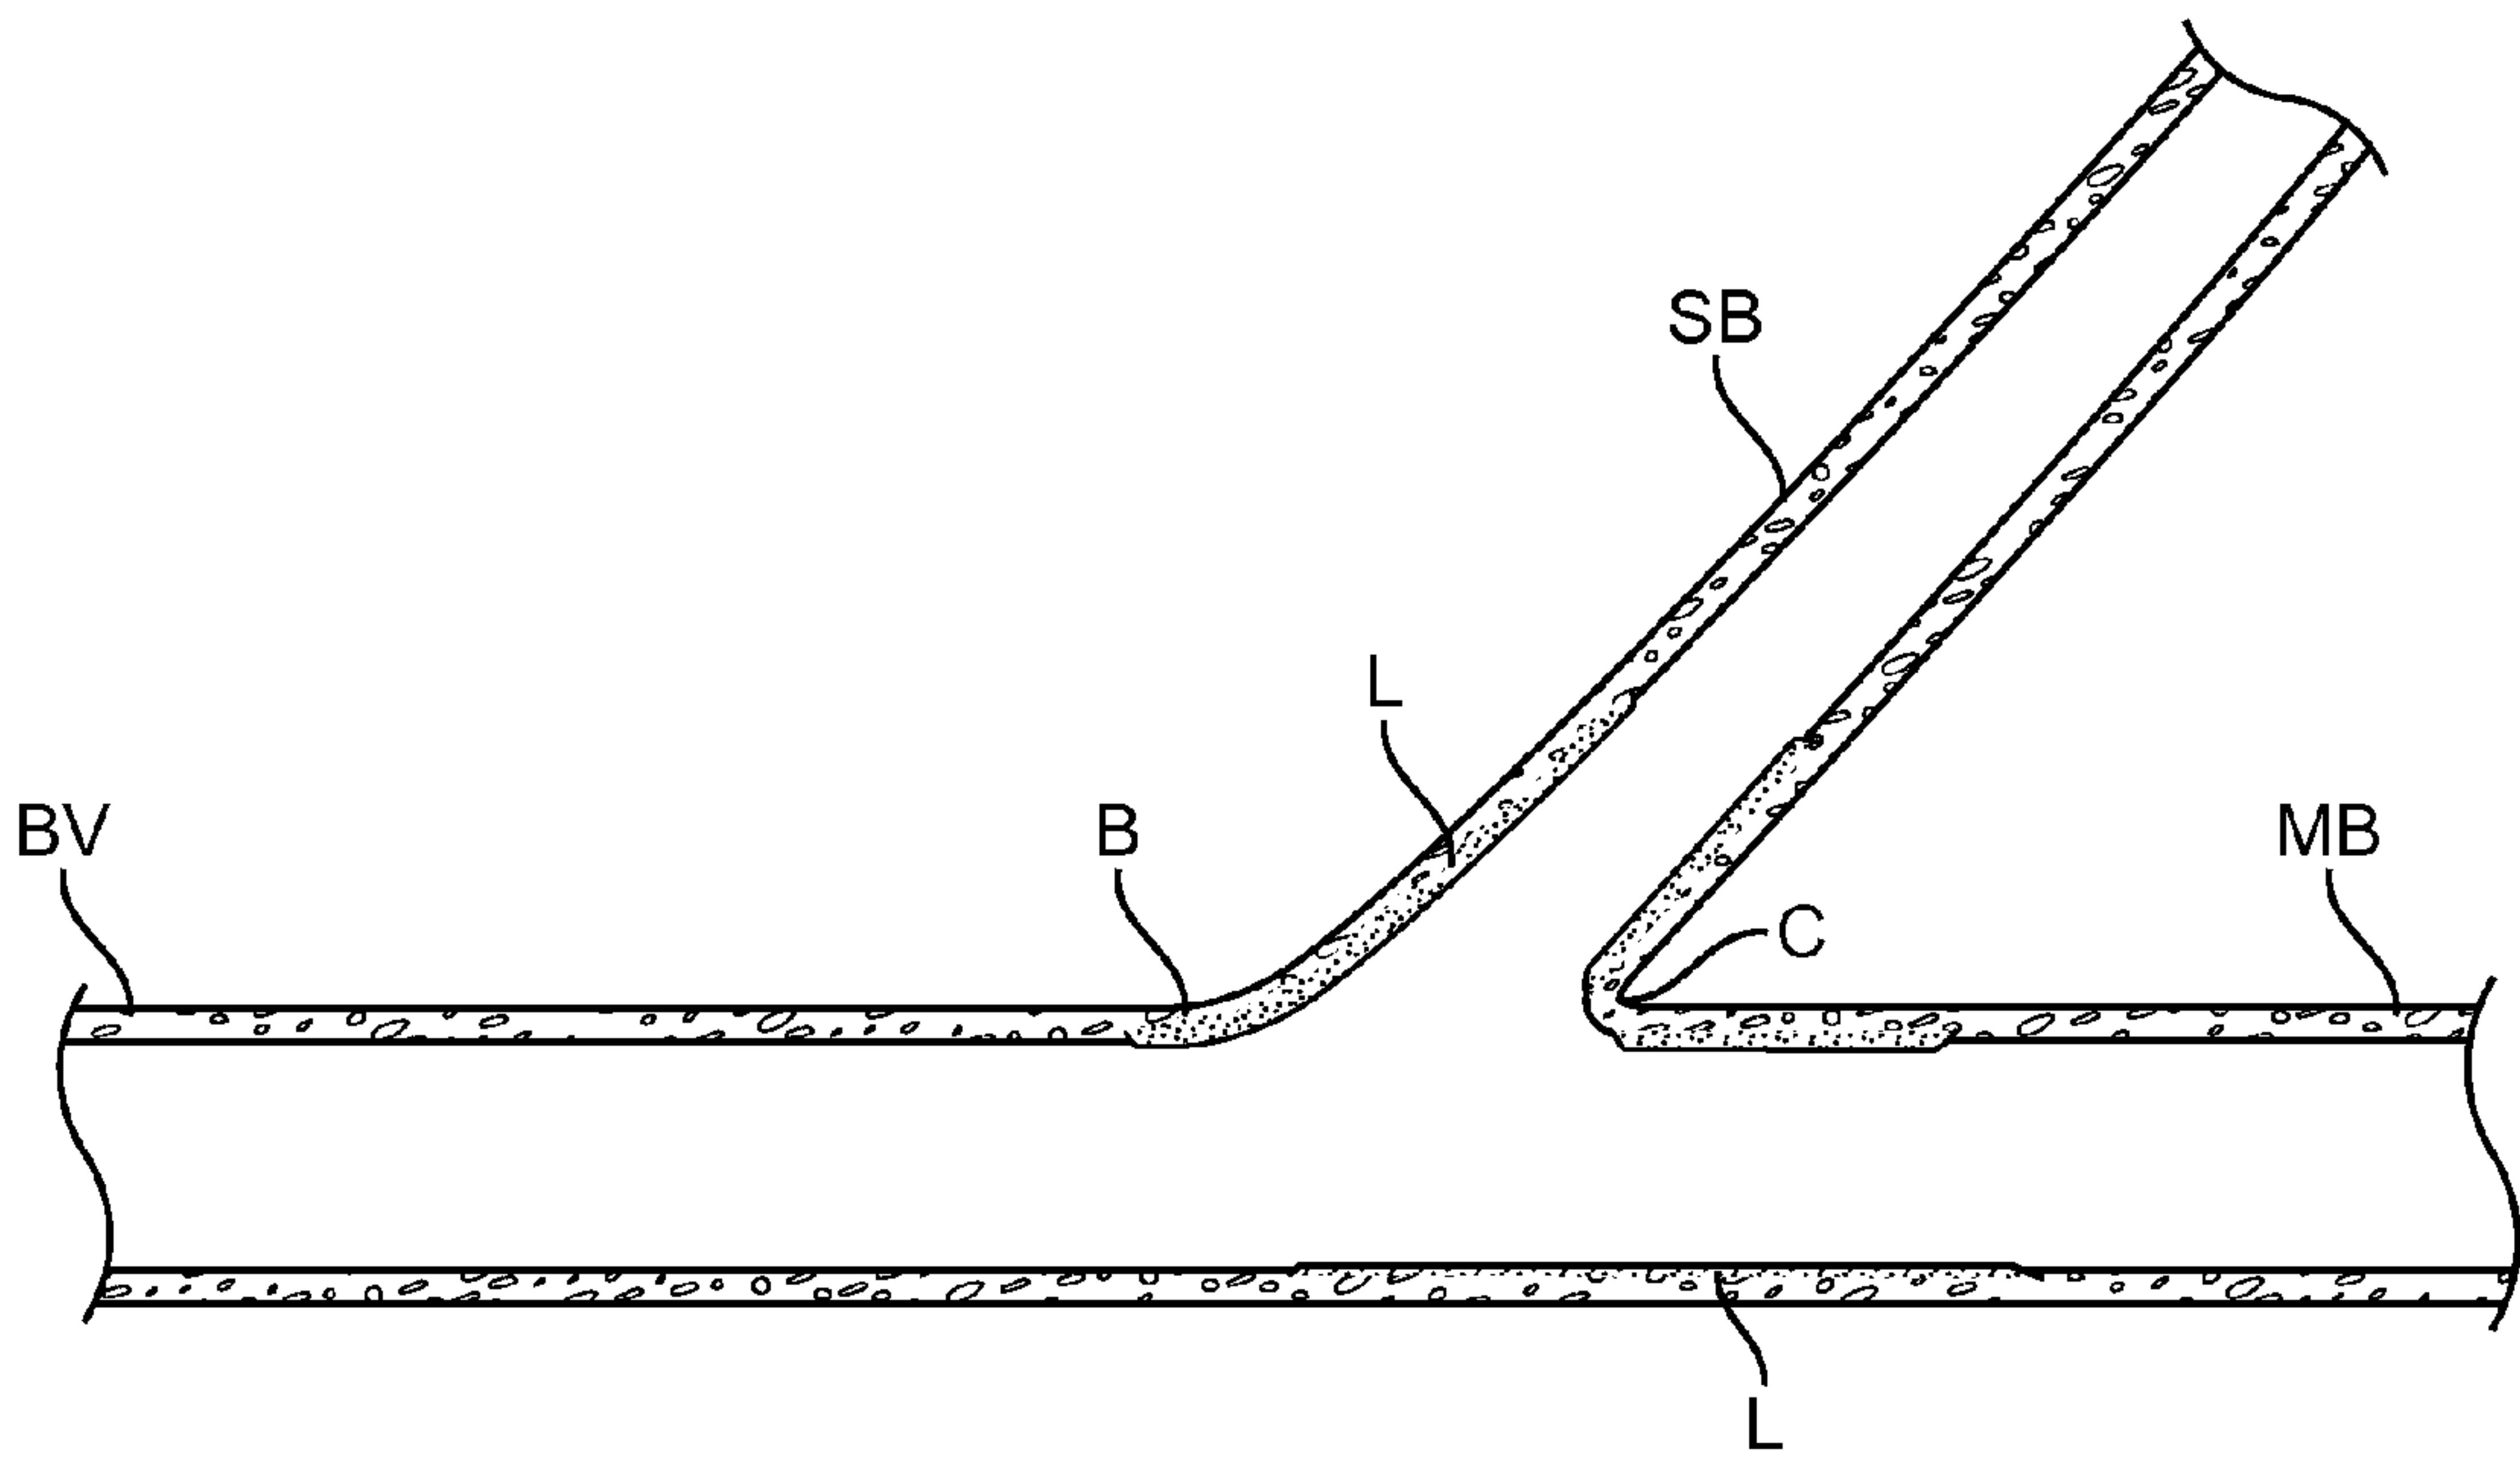


FIG. 4J

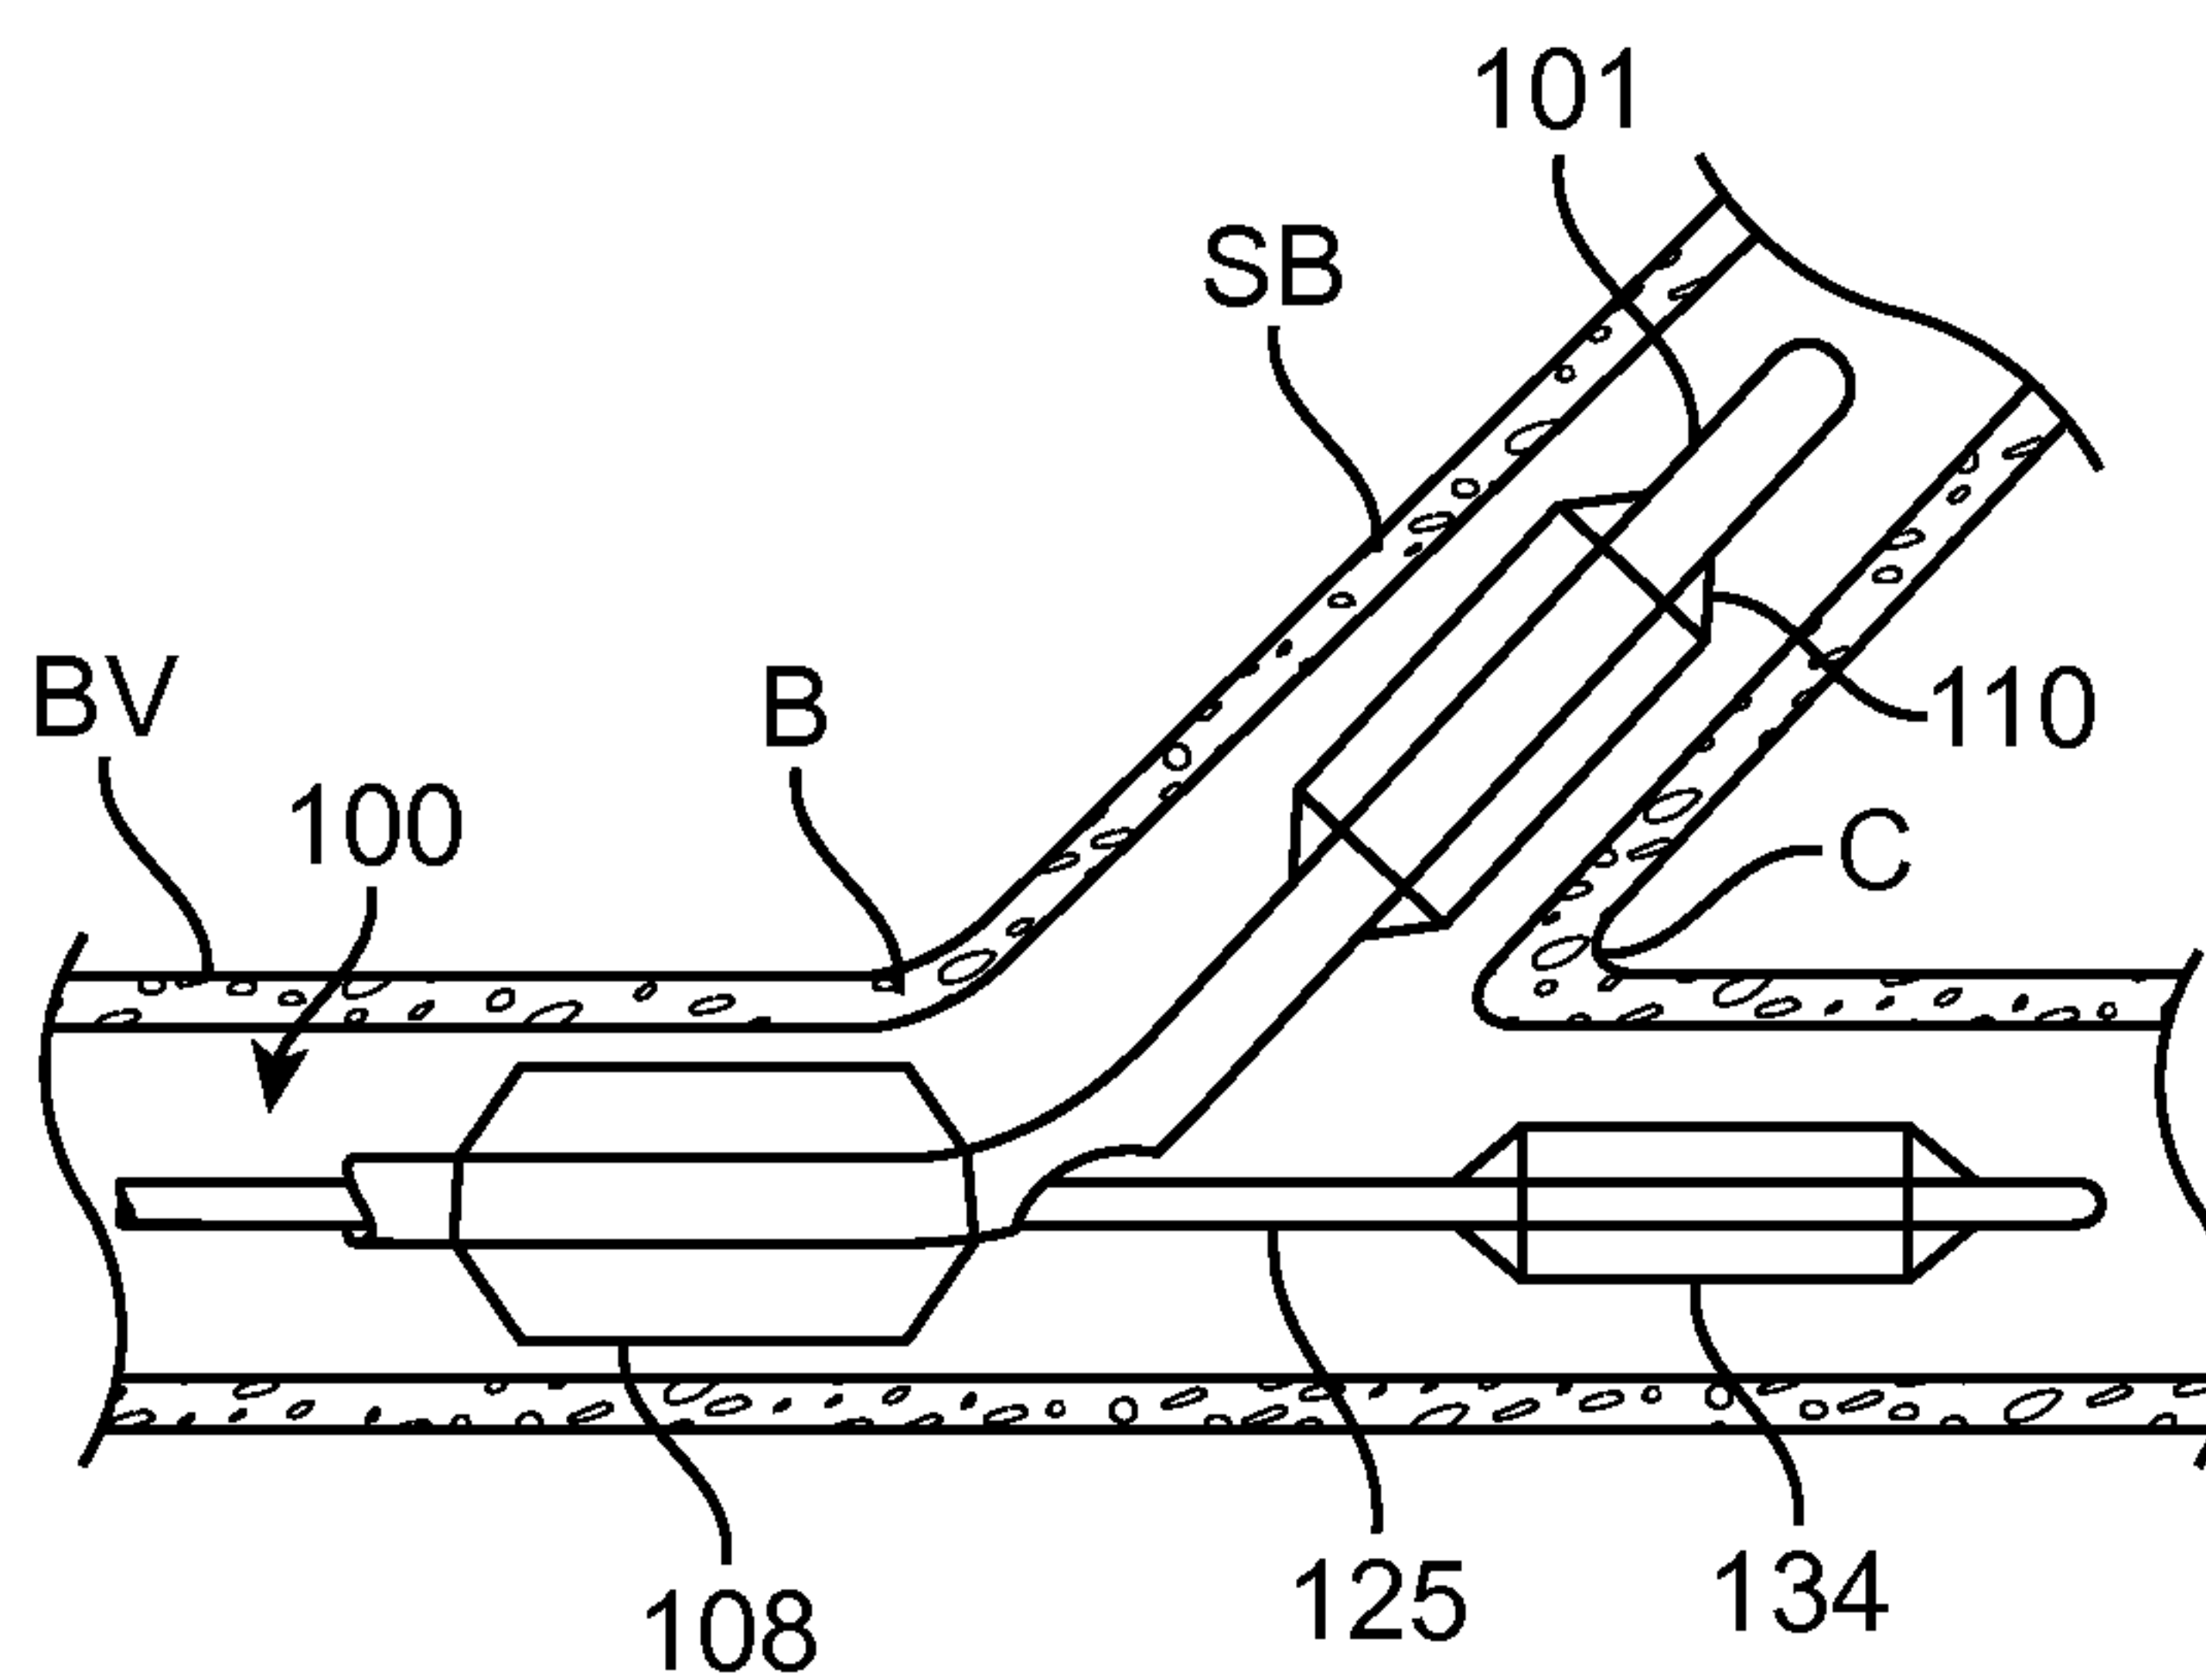


FIG. 5

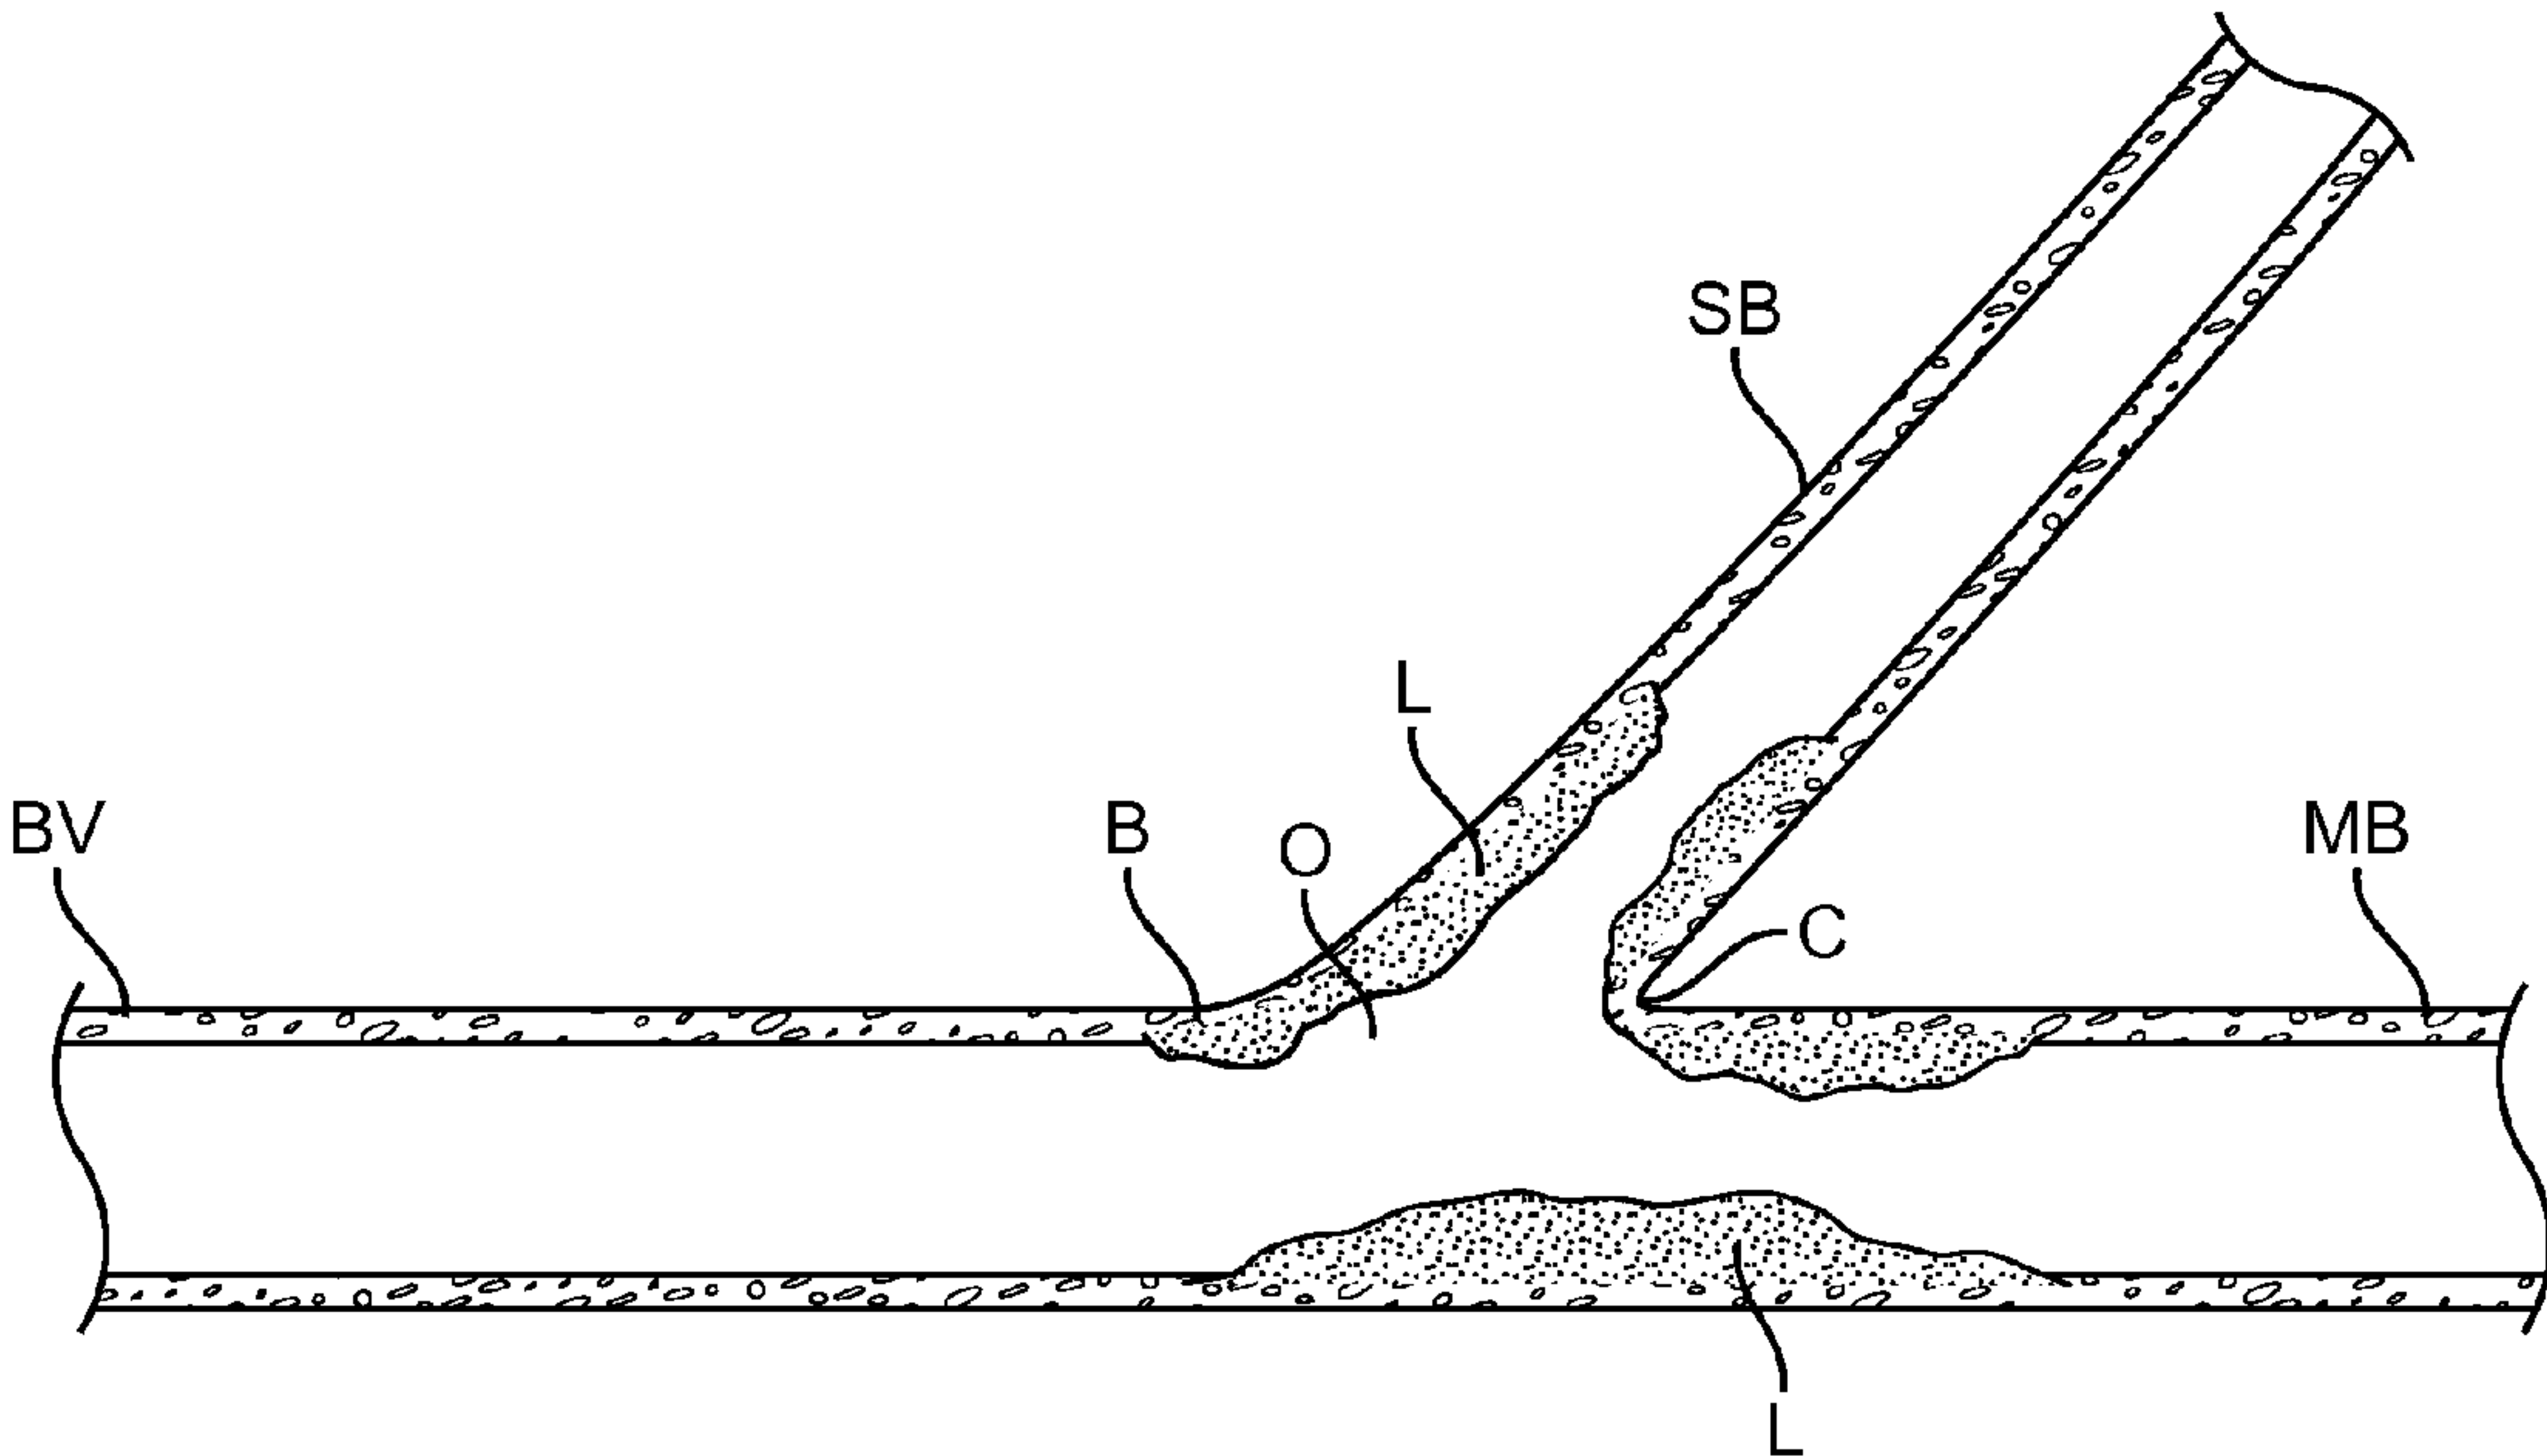


FIG. 6A

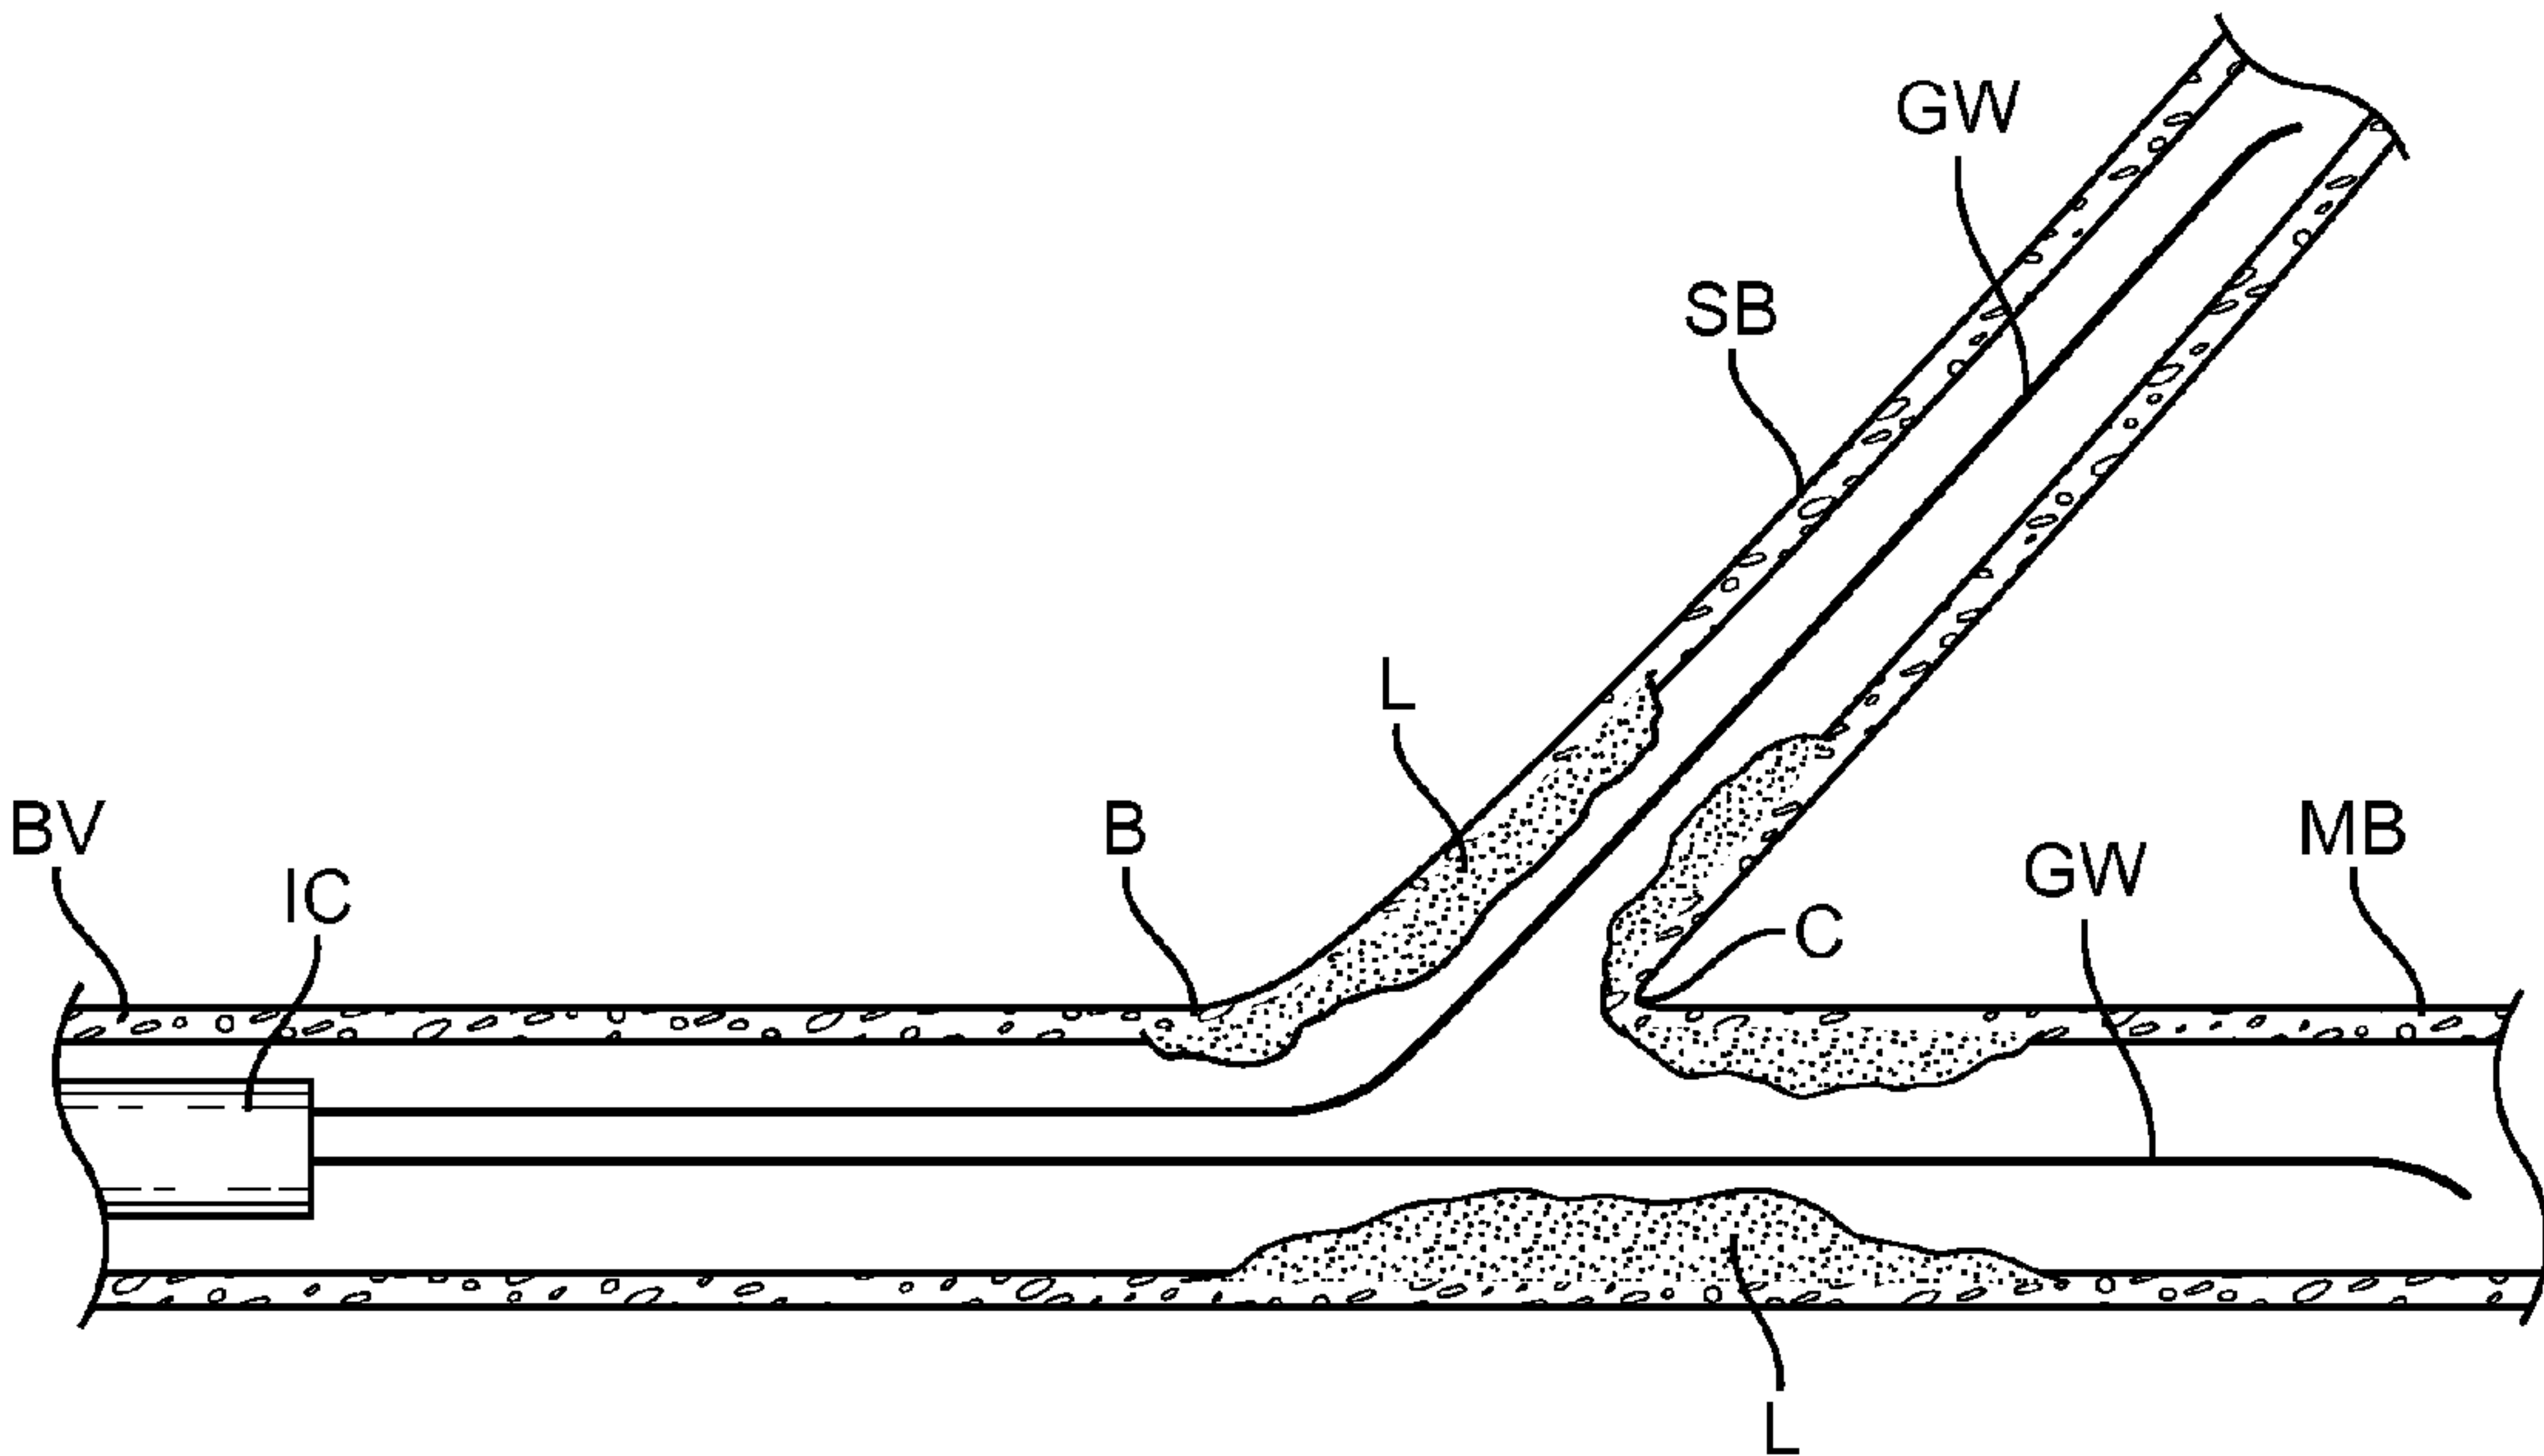


FIG. 6B

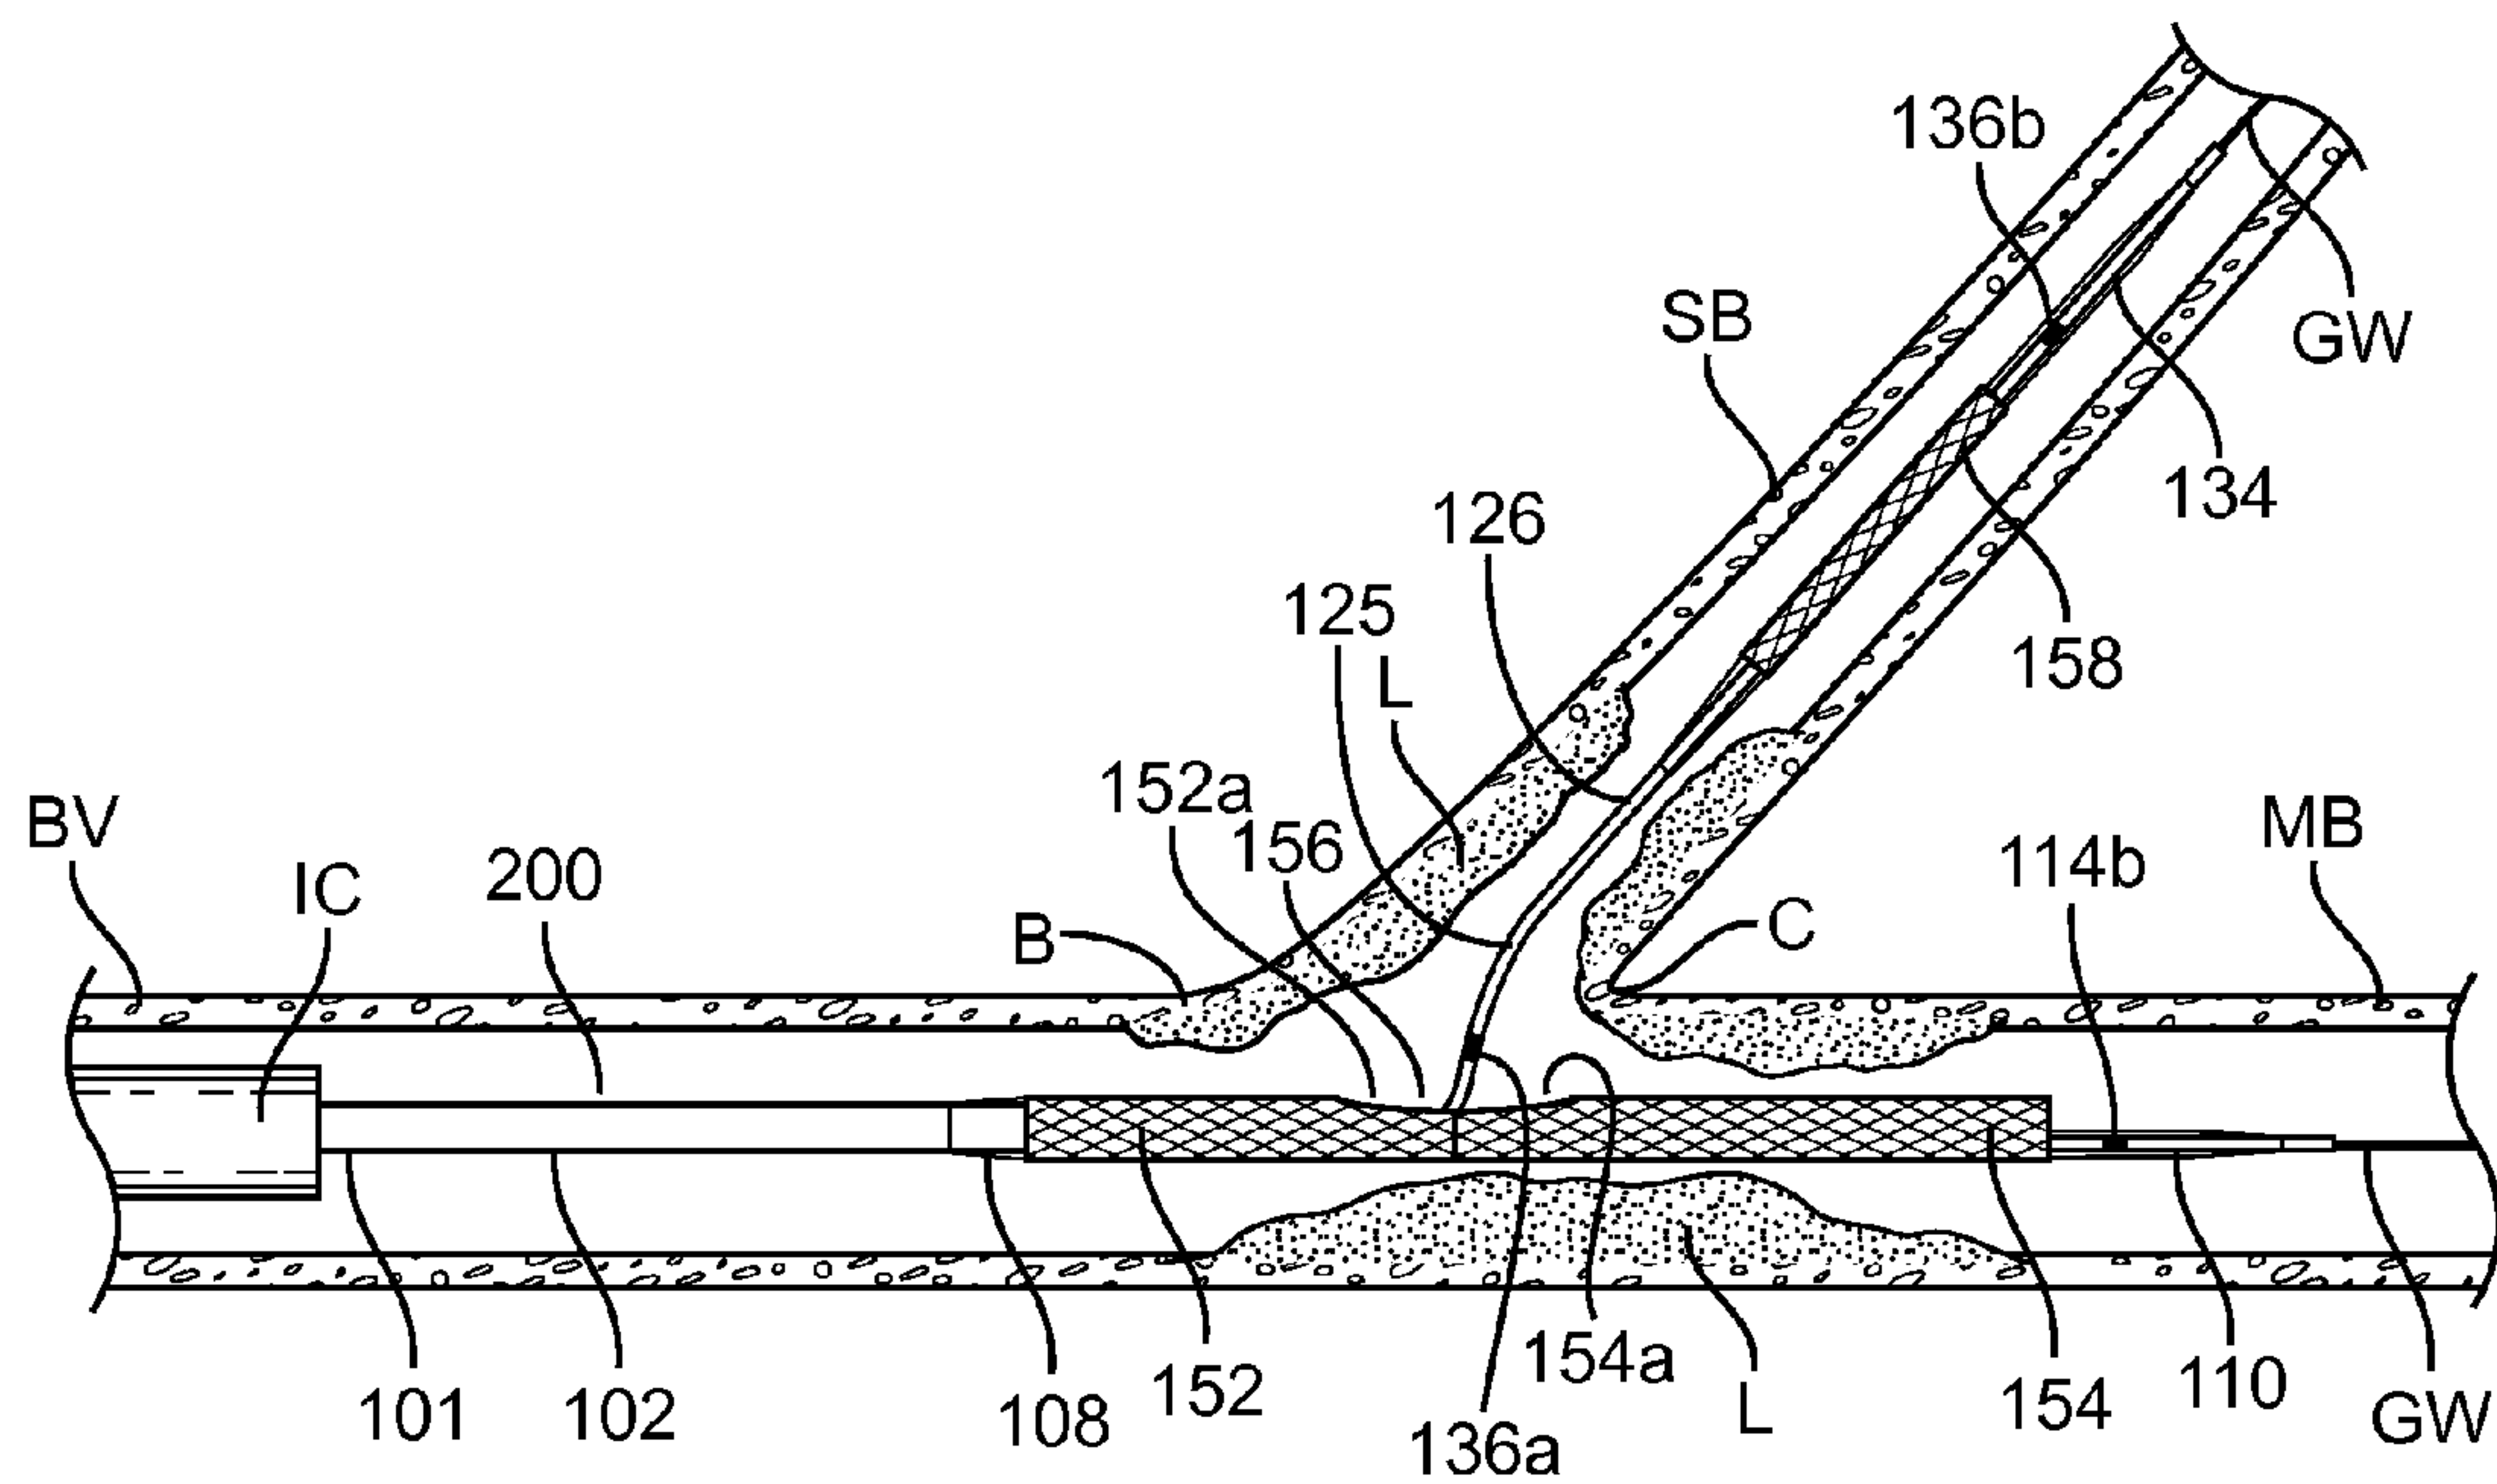


FIG. 6C

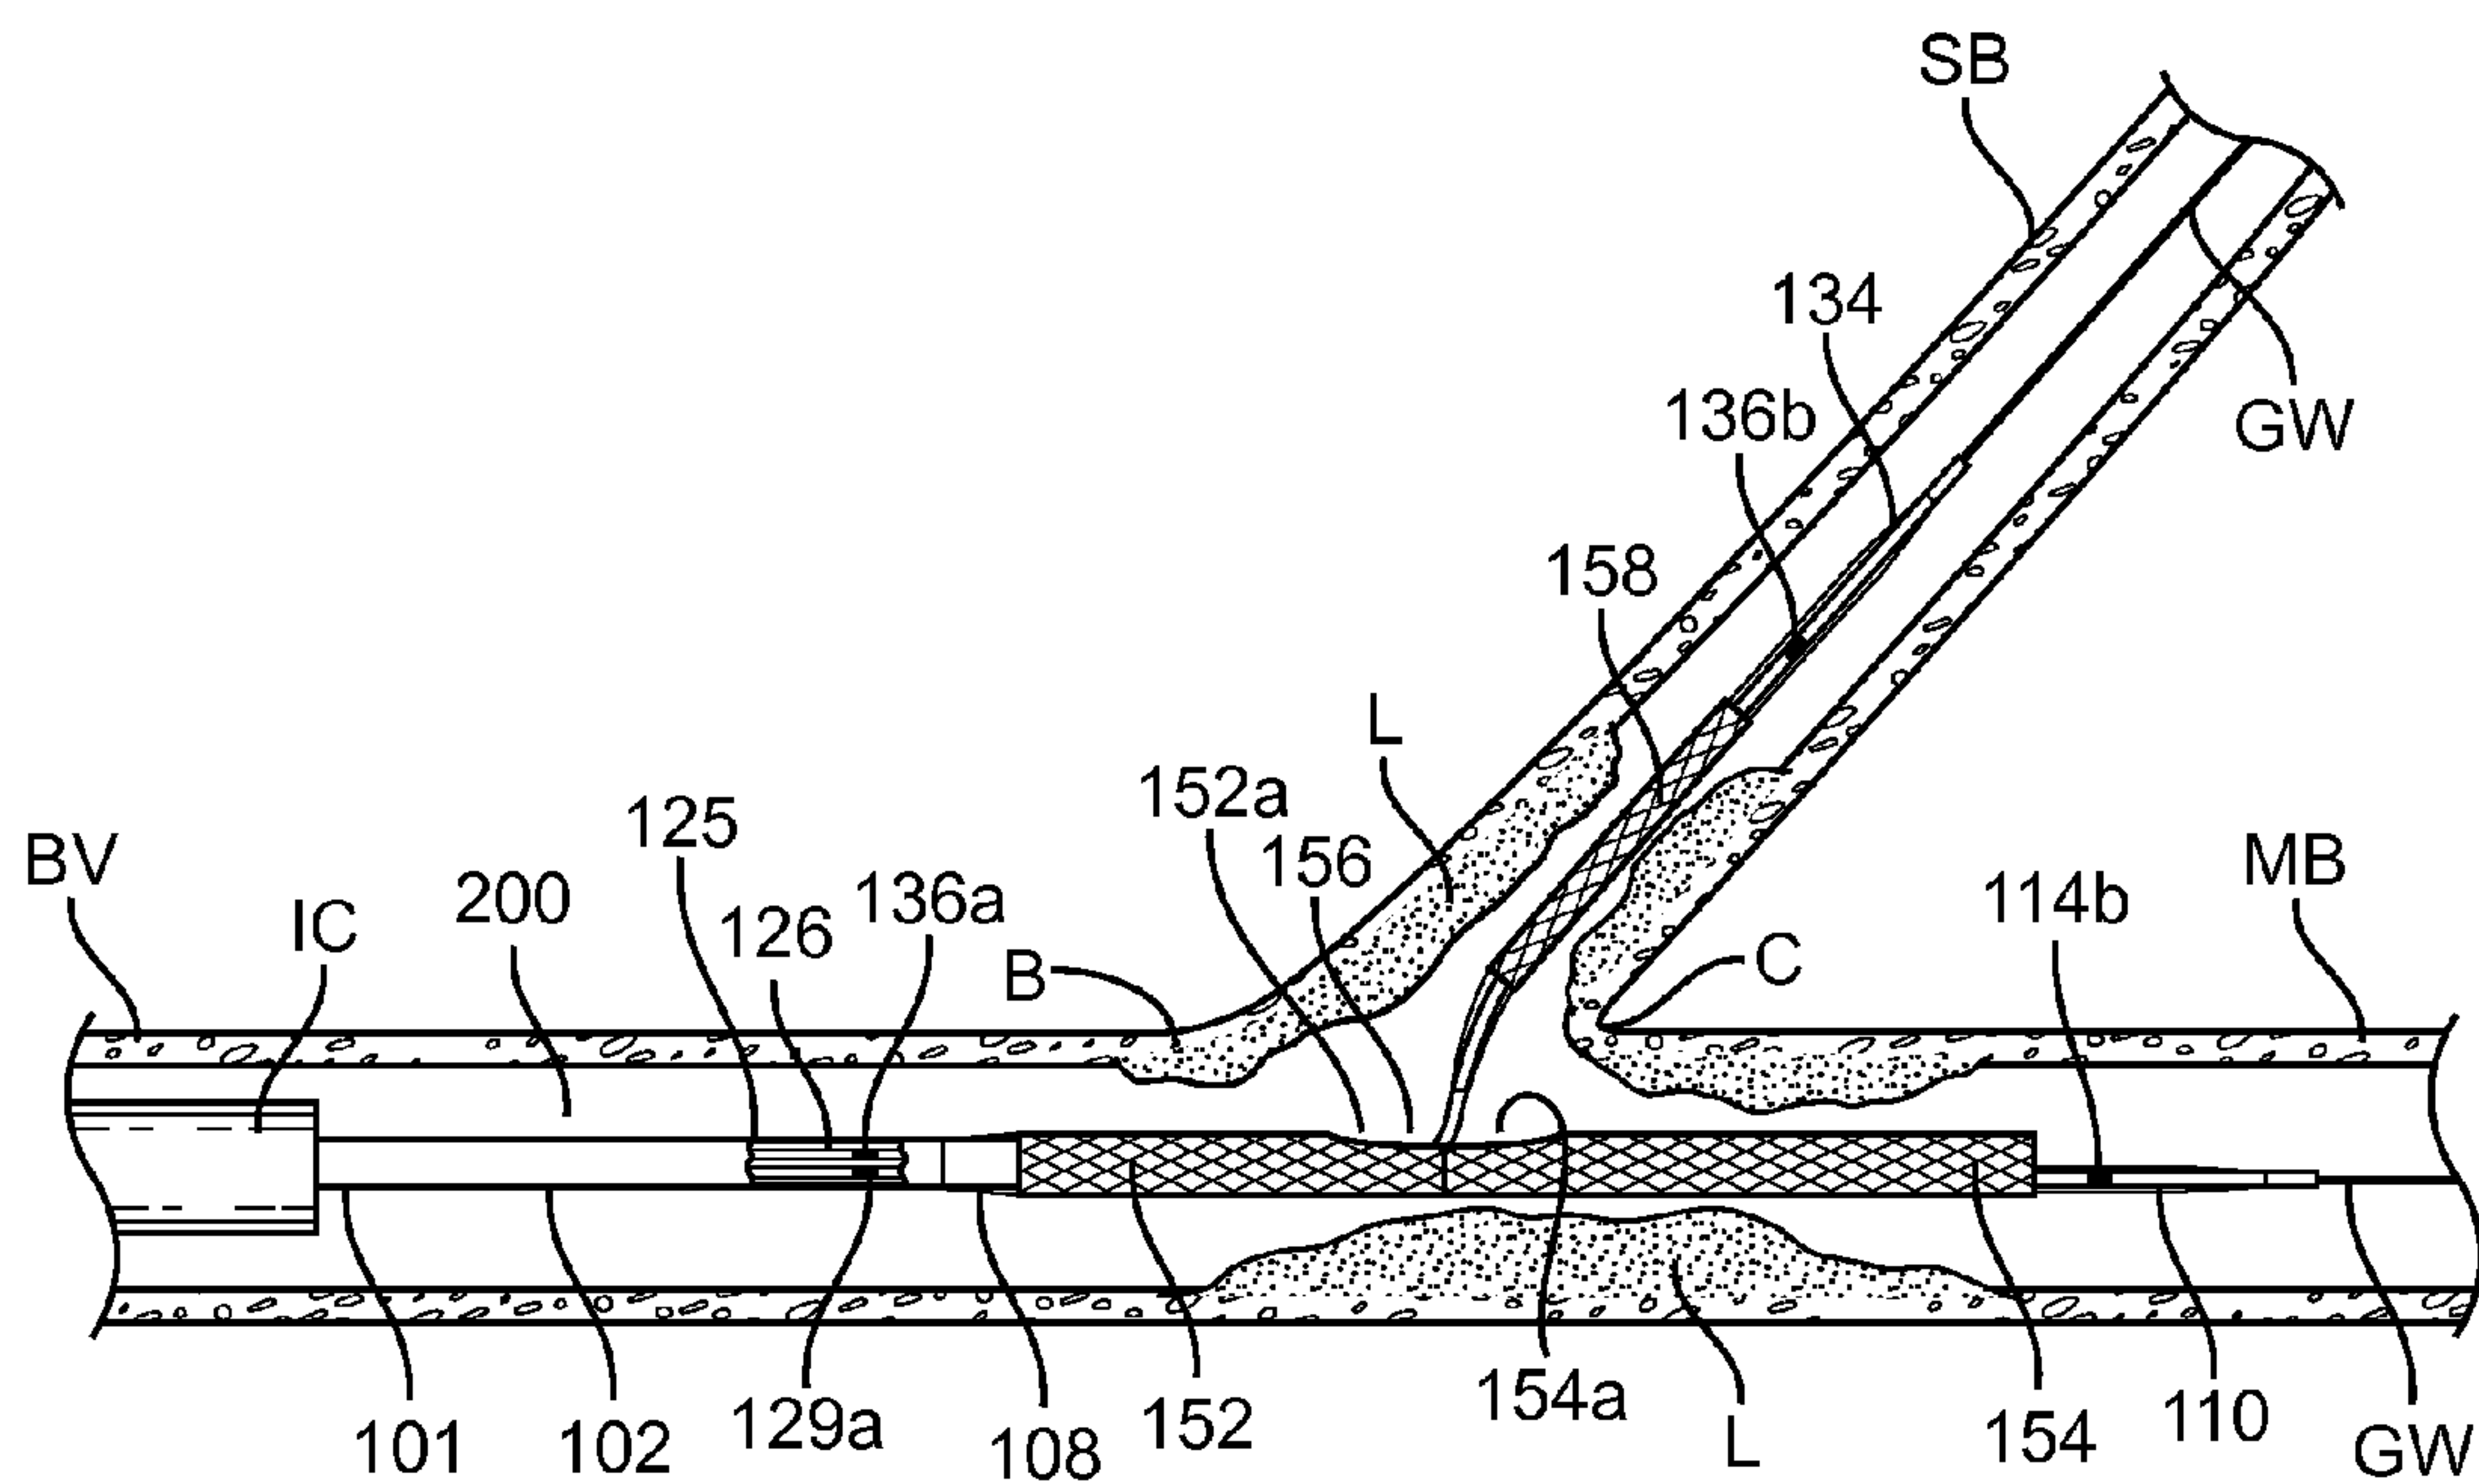


FIG. 6D

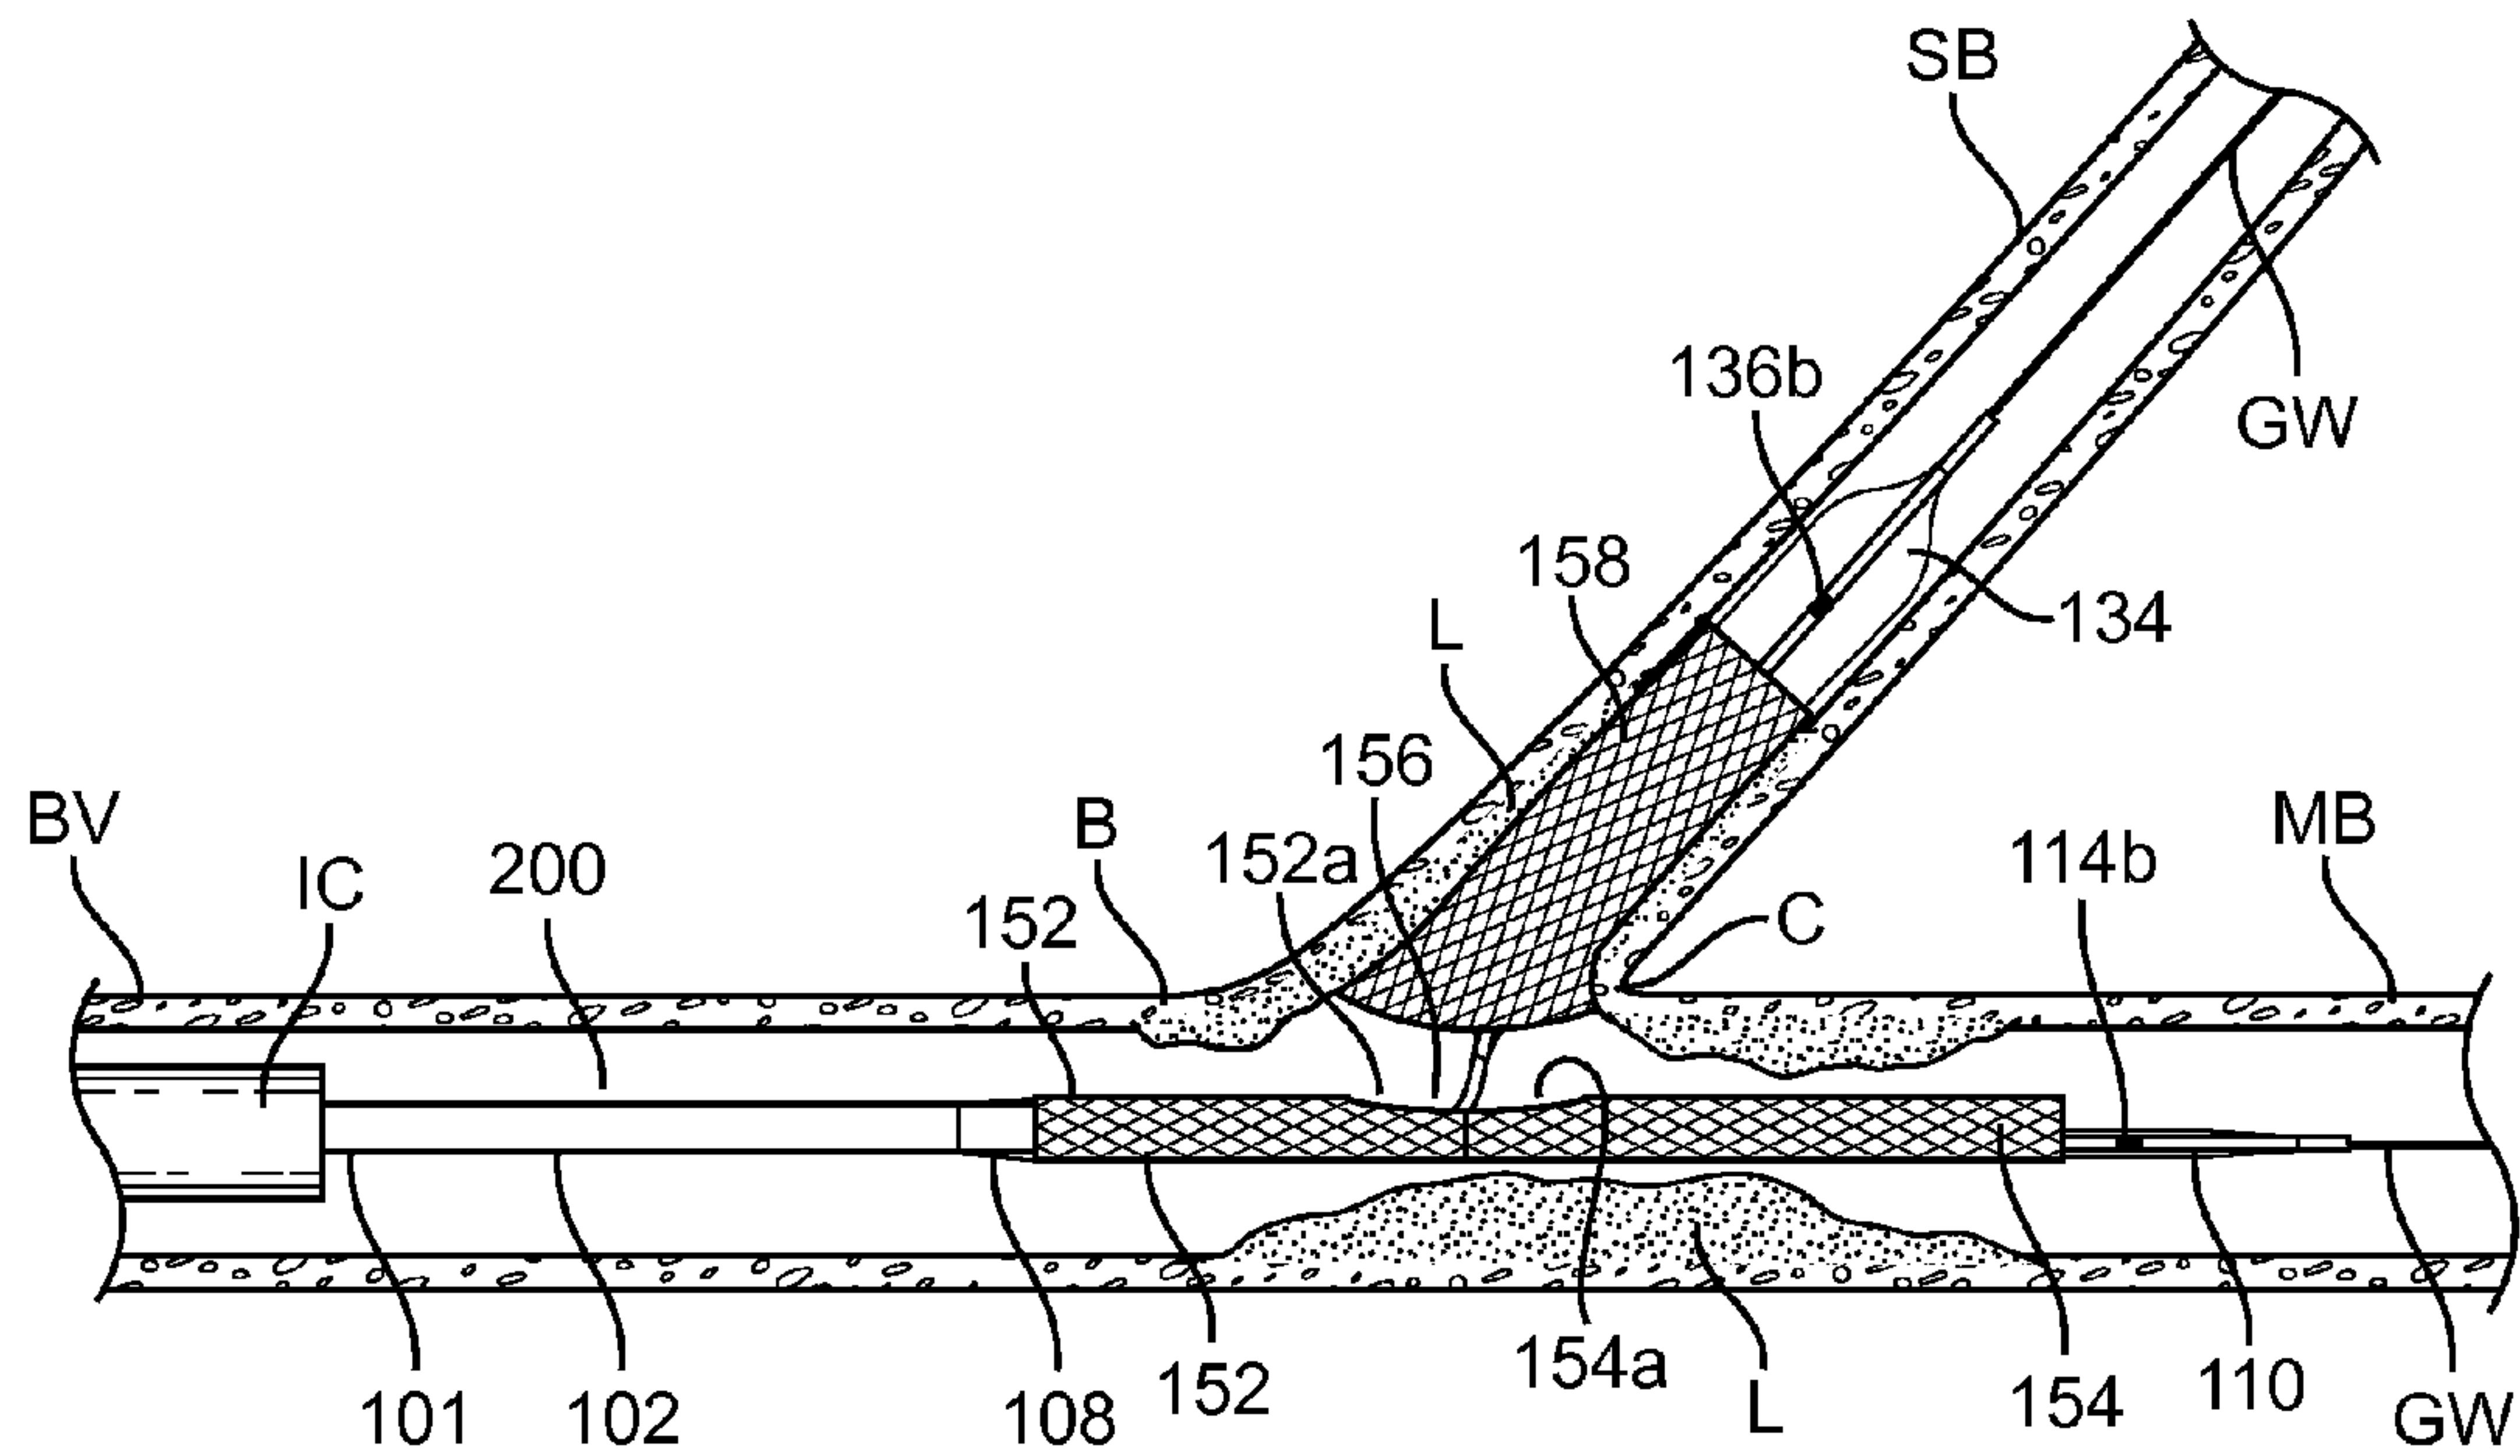


FIG. 6E

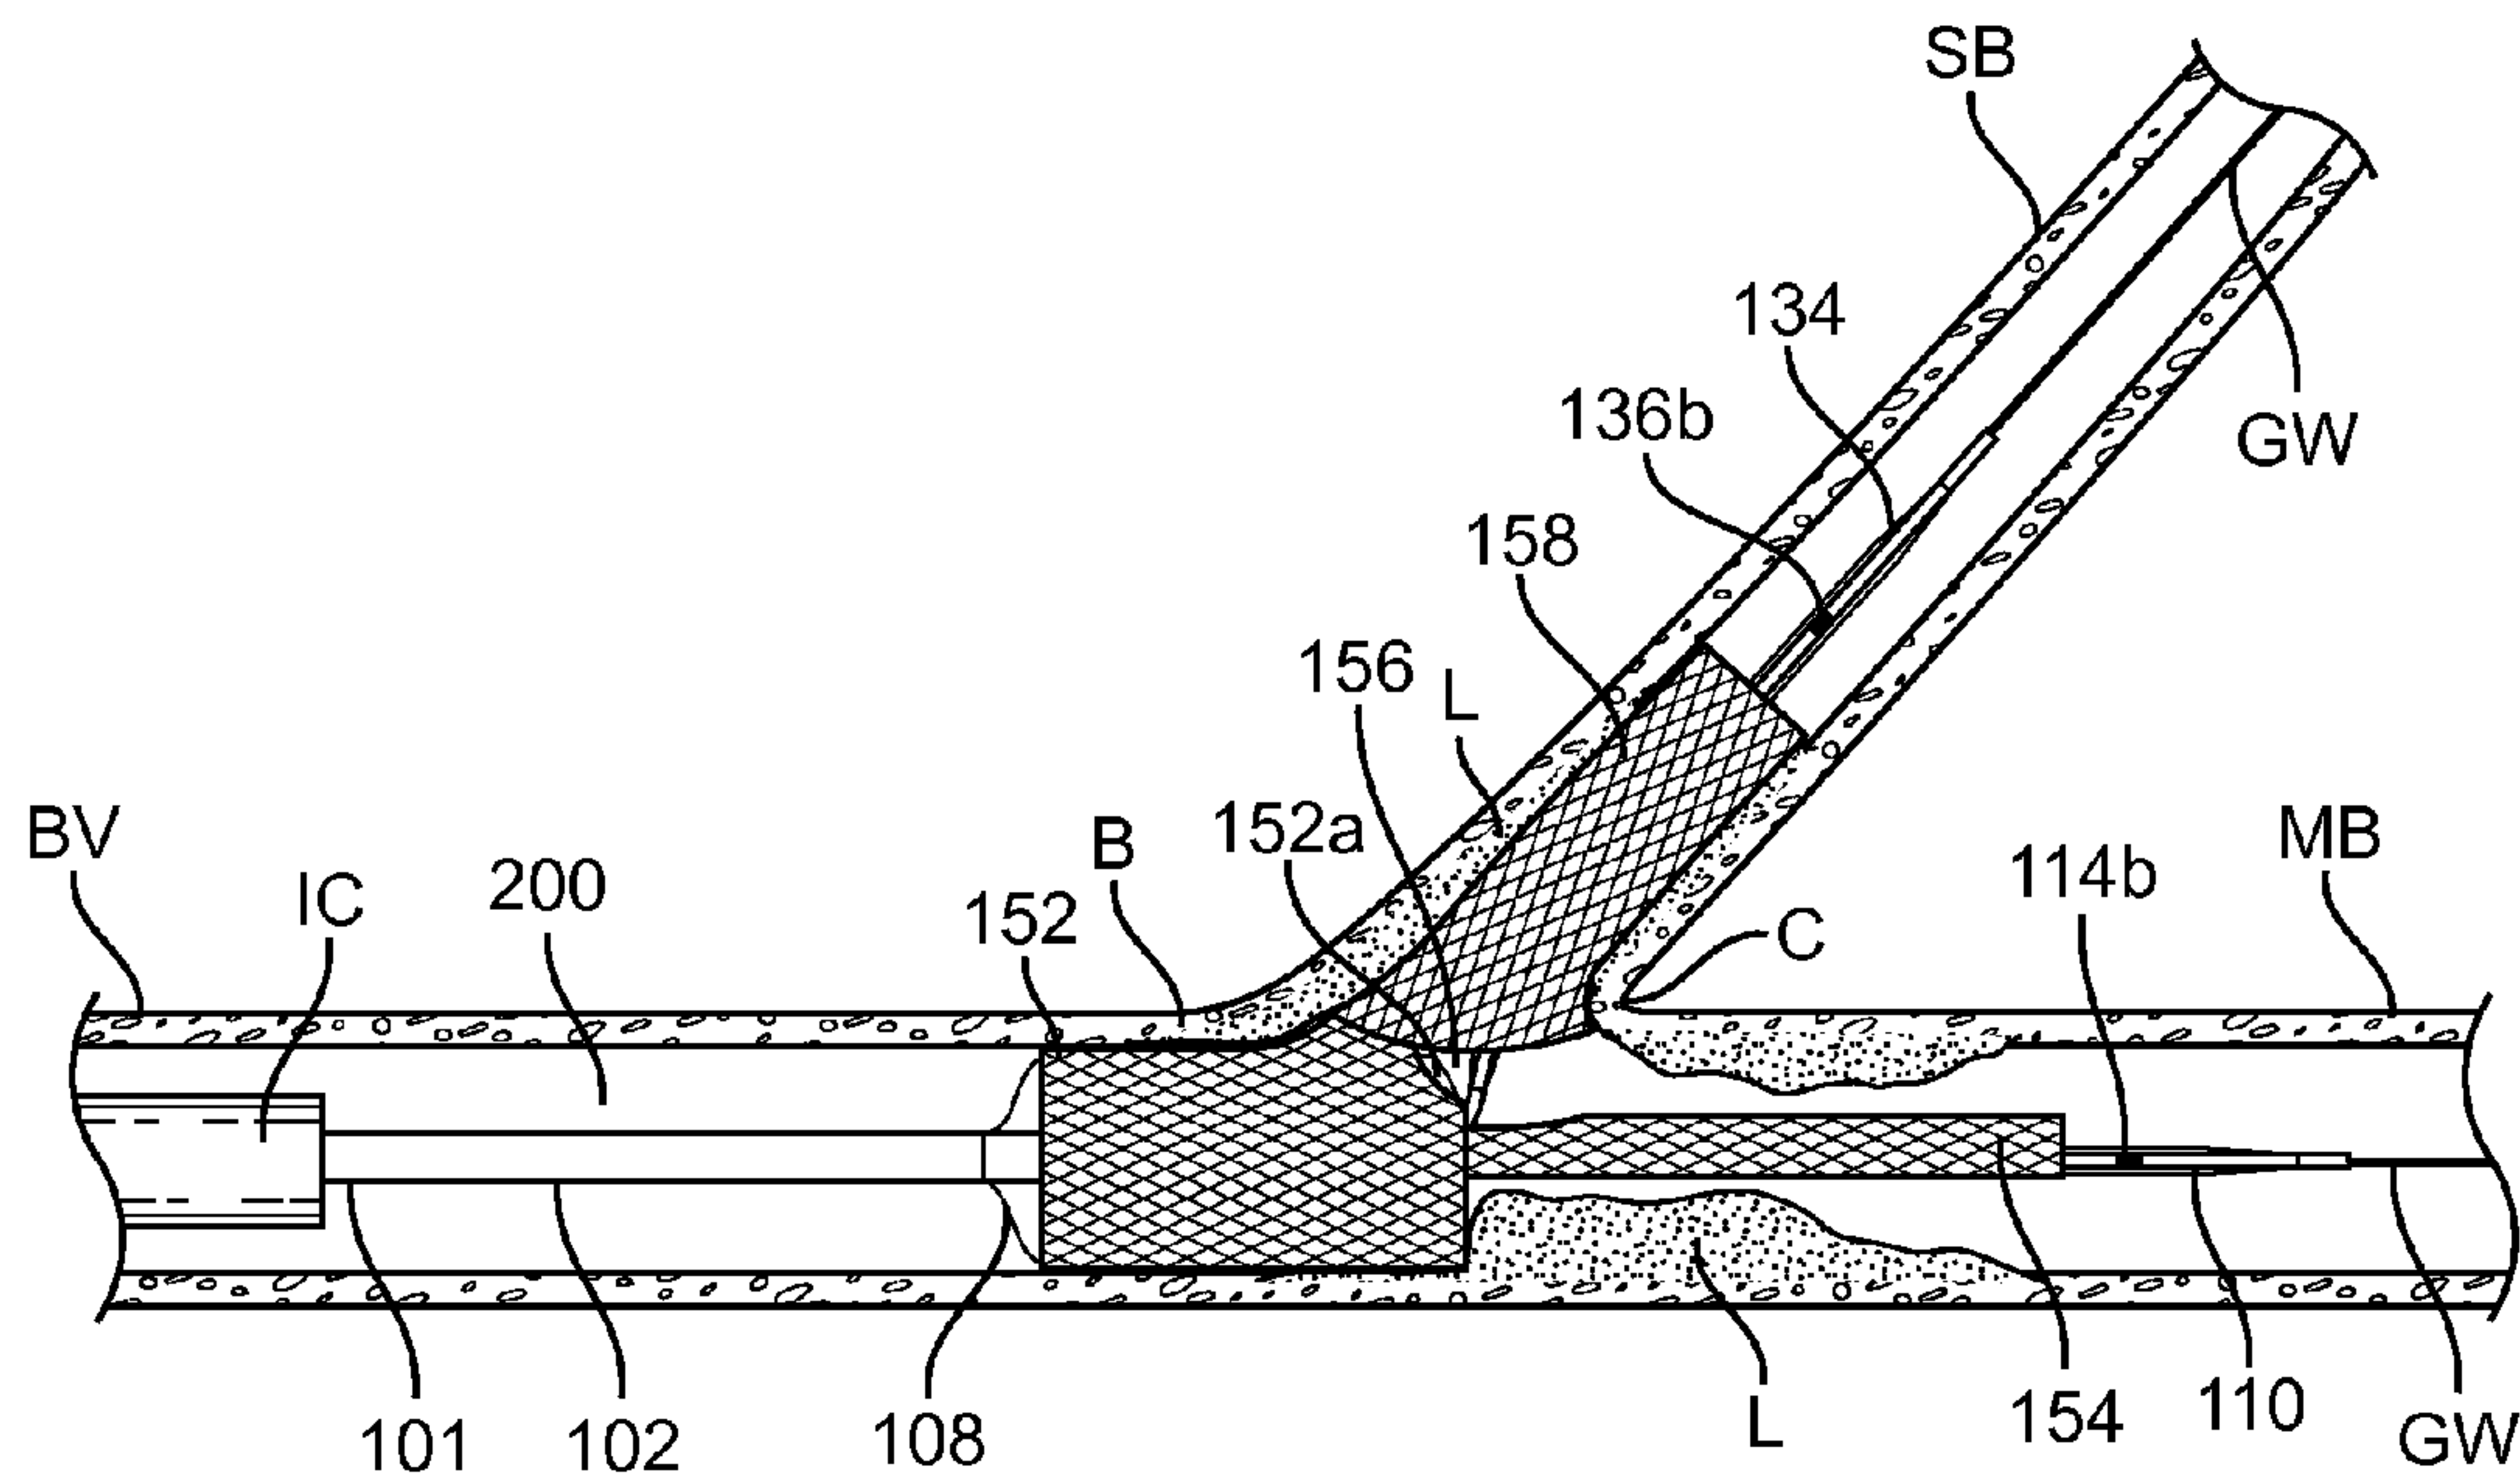


FIG. 6F

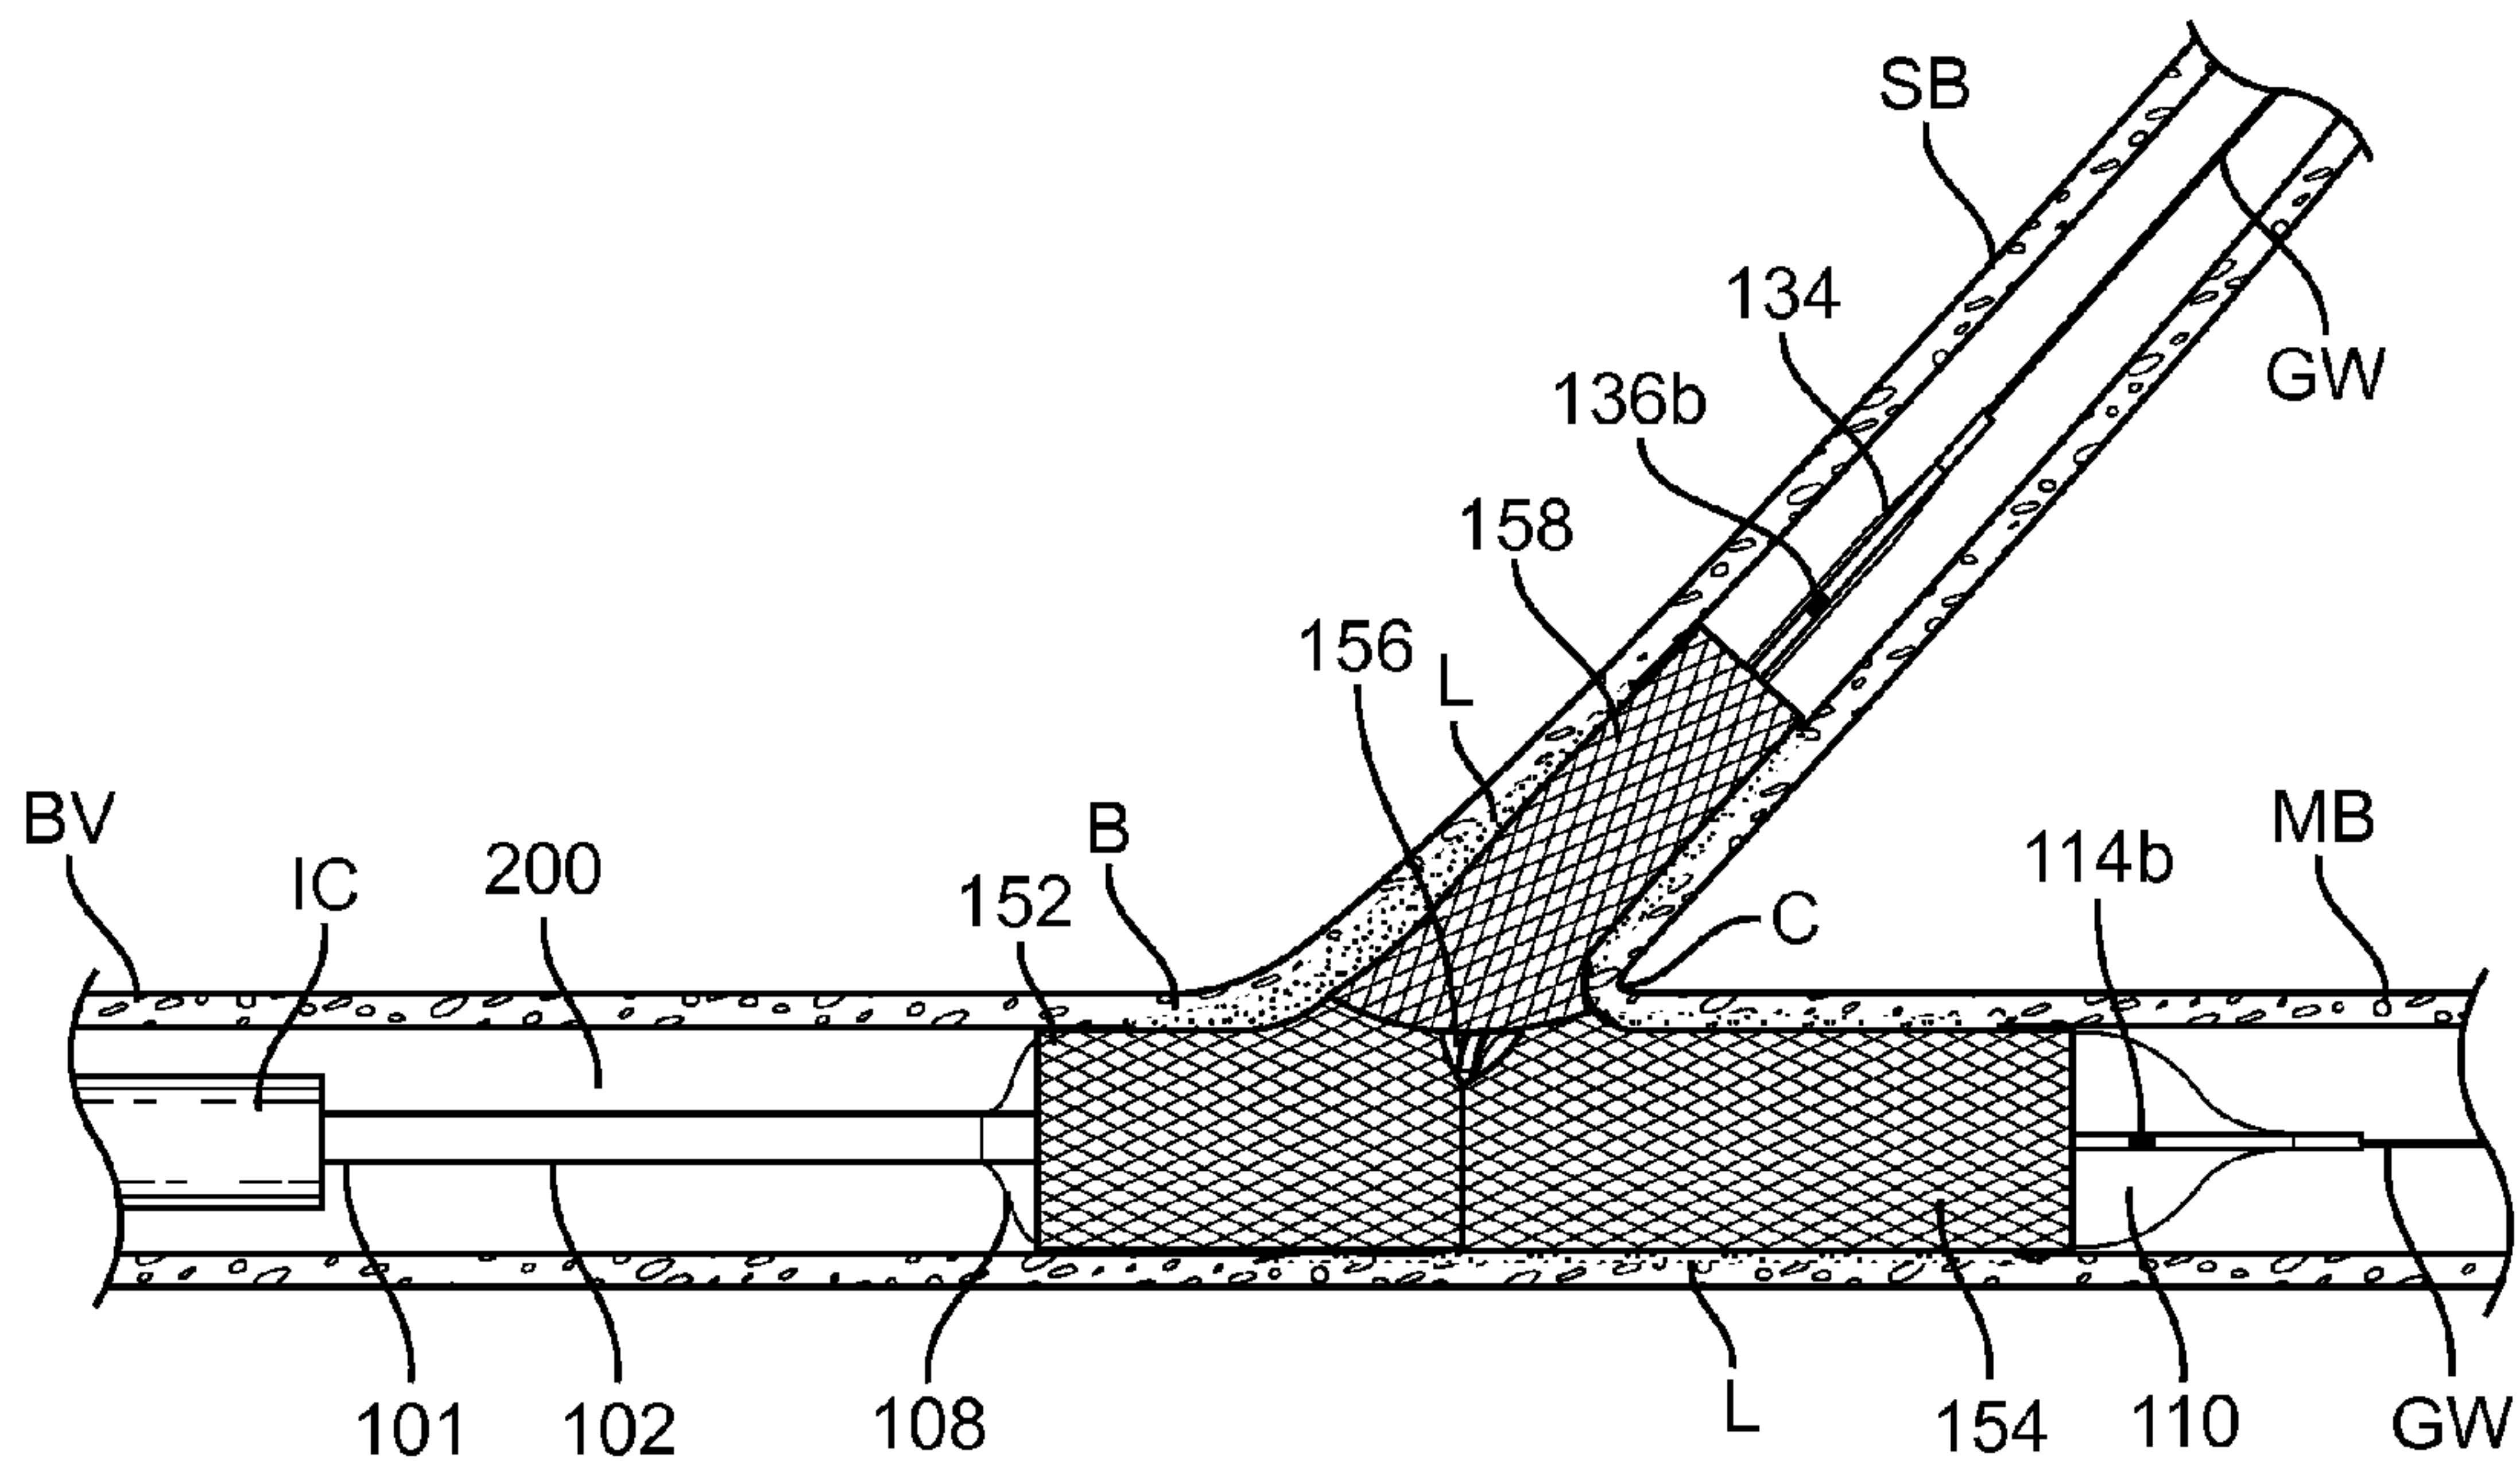


FIG. 6G

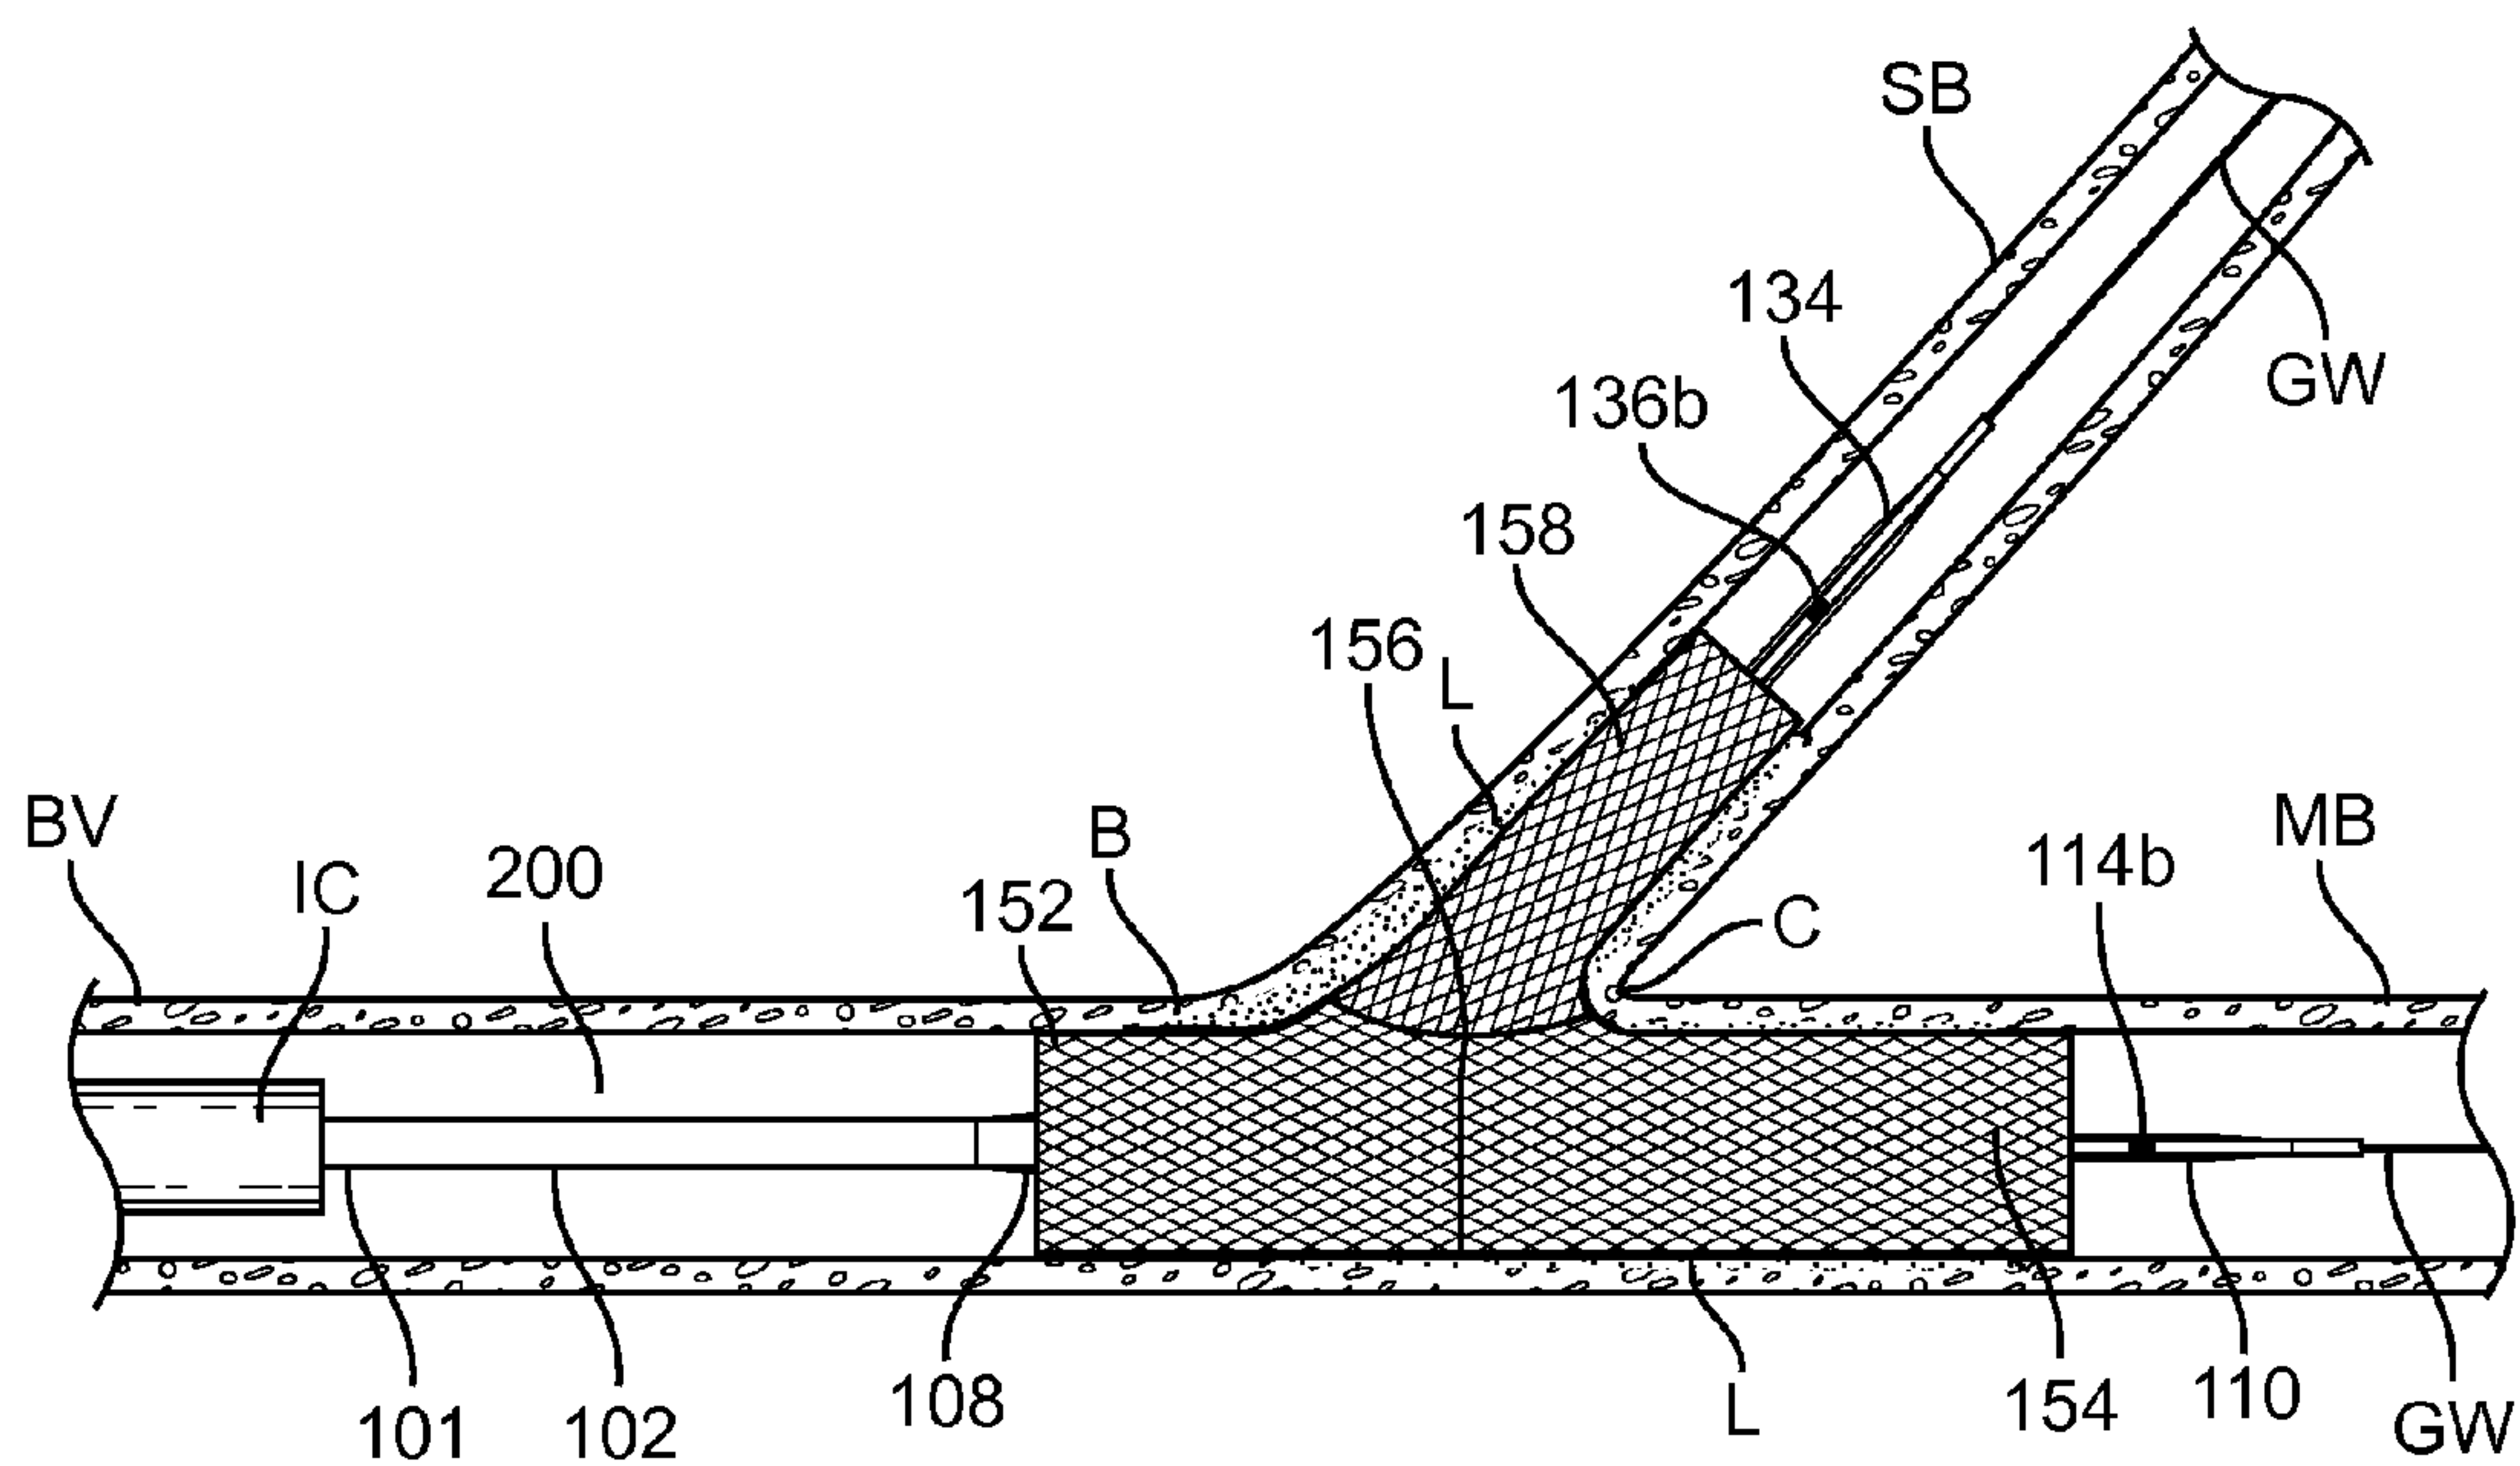


FIG. 6H

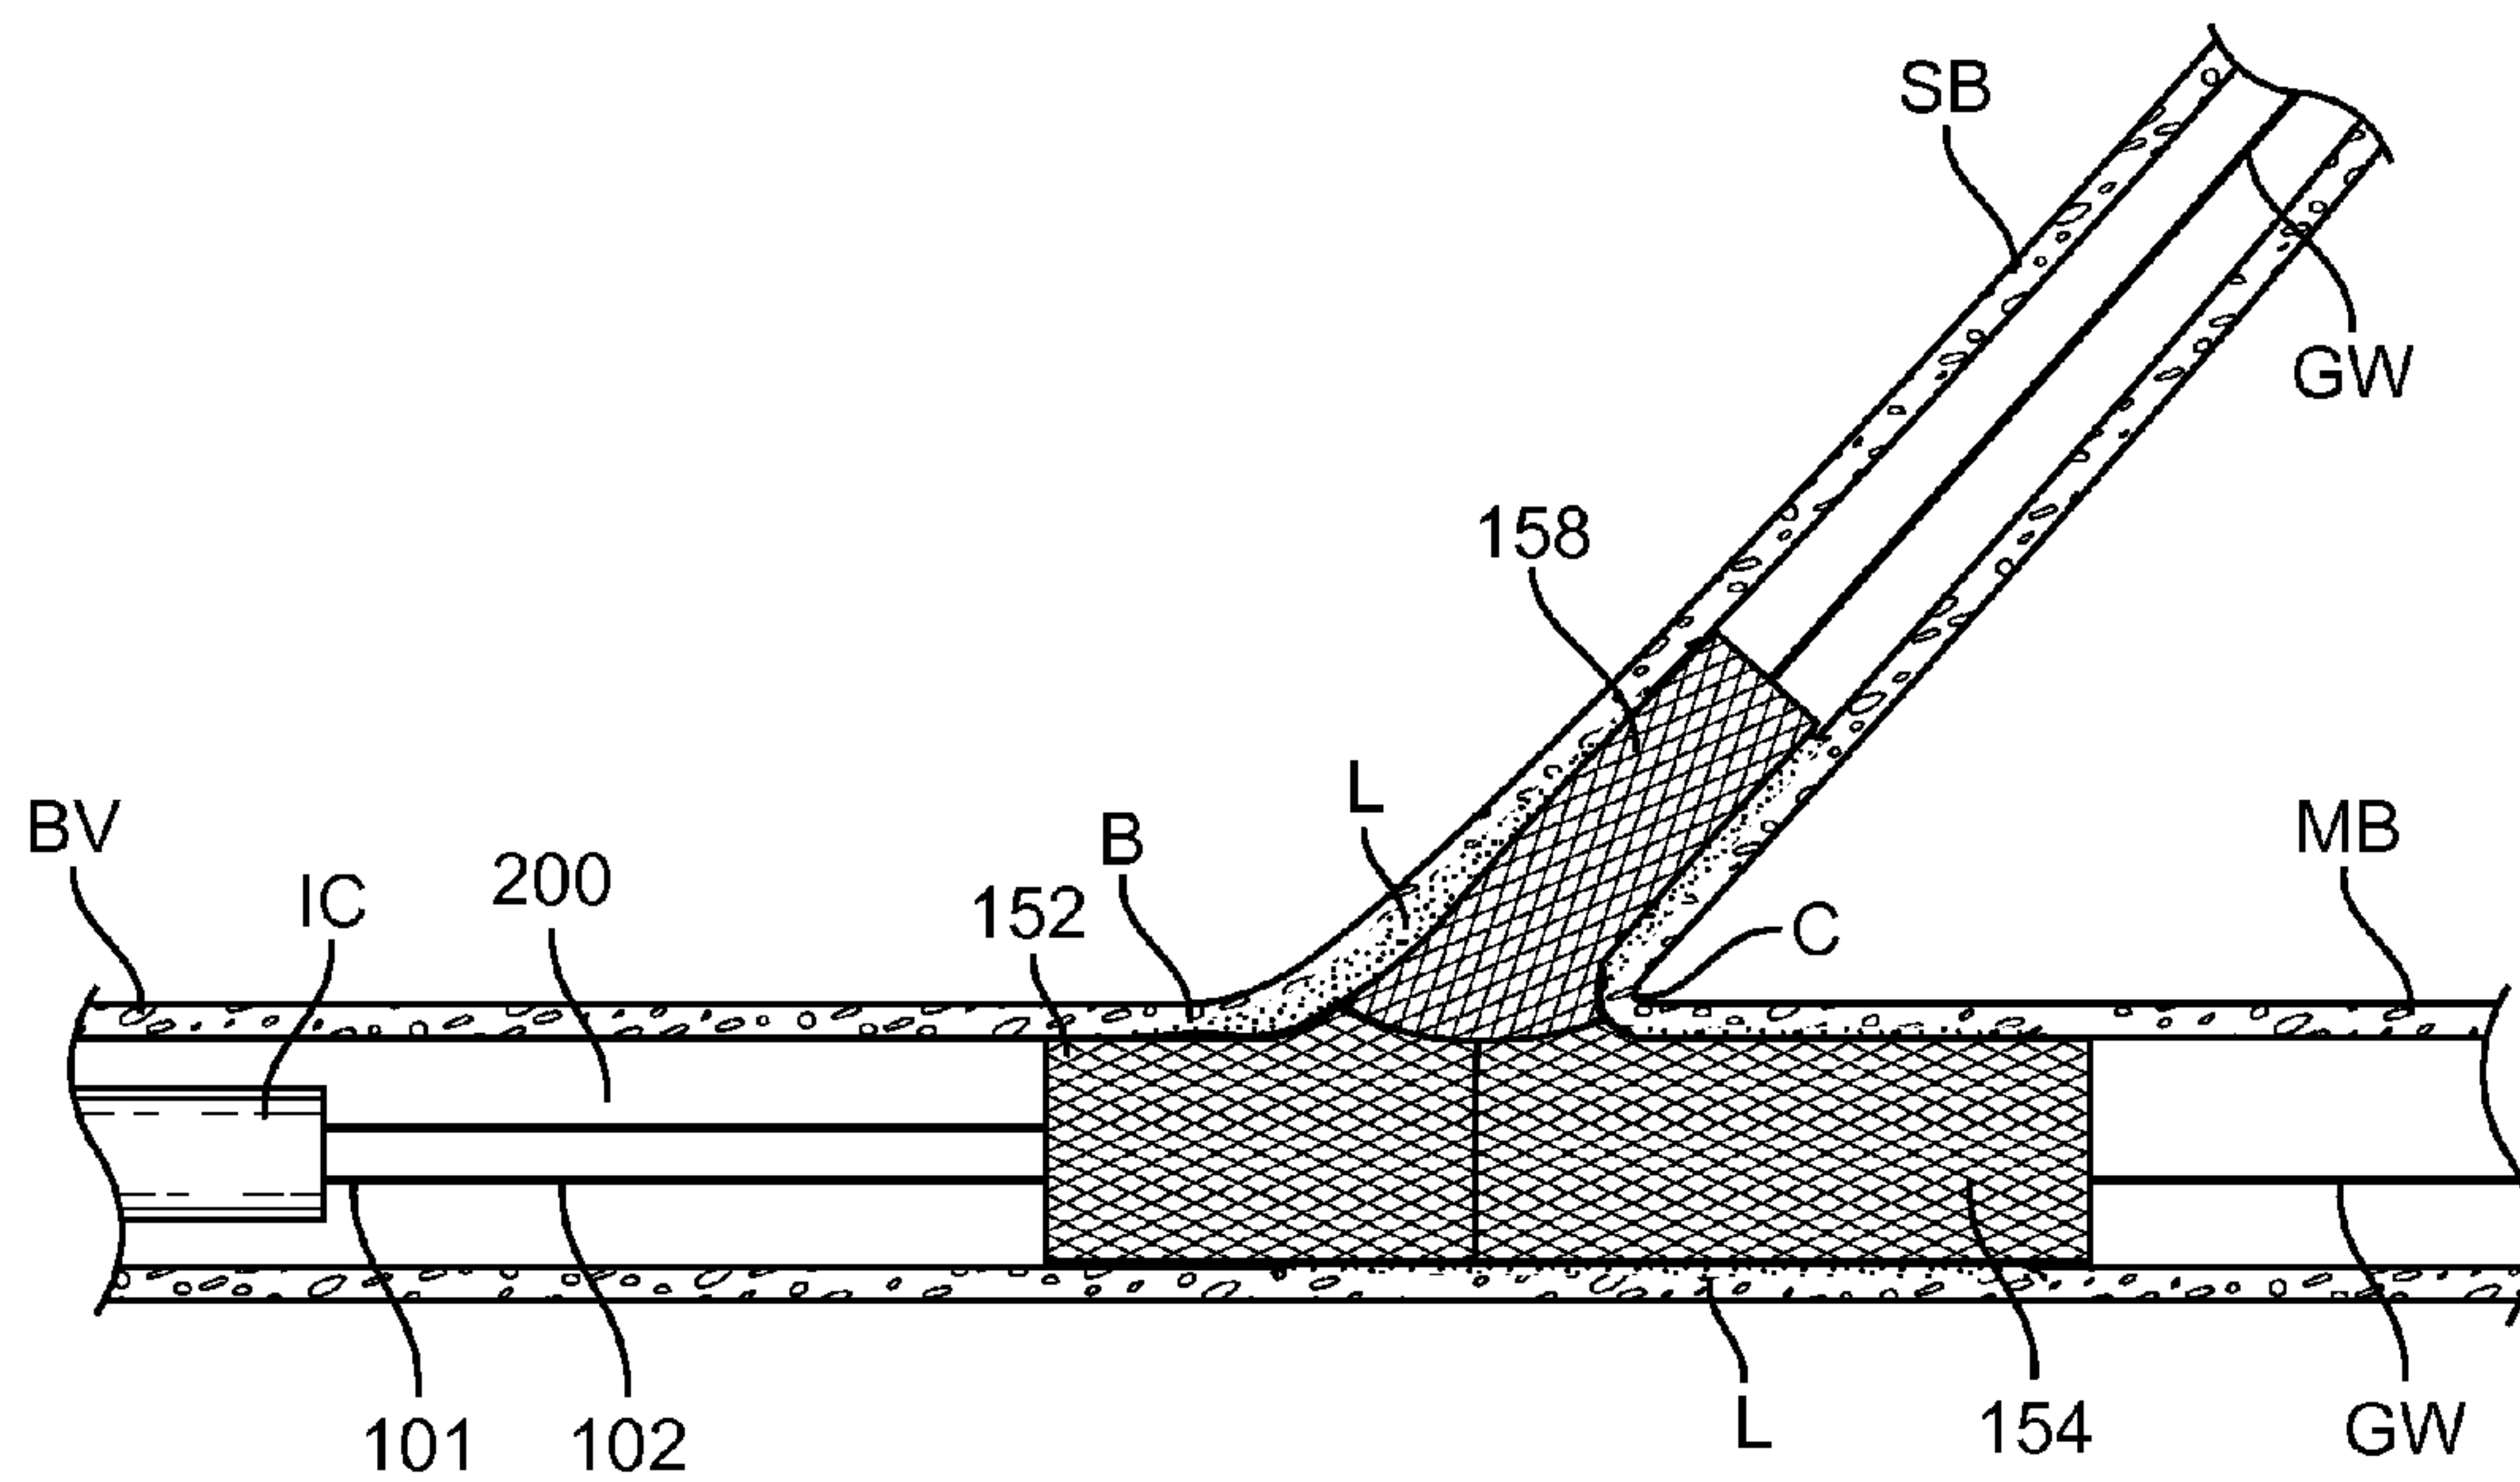


FIG. 6I

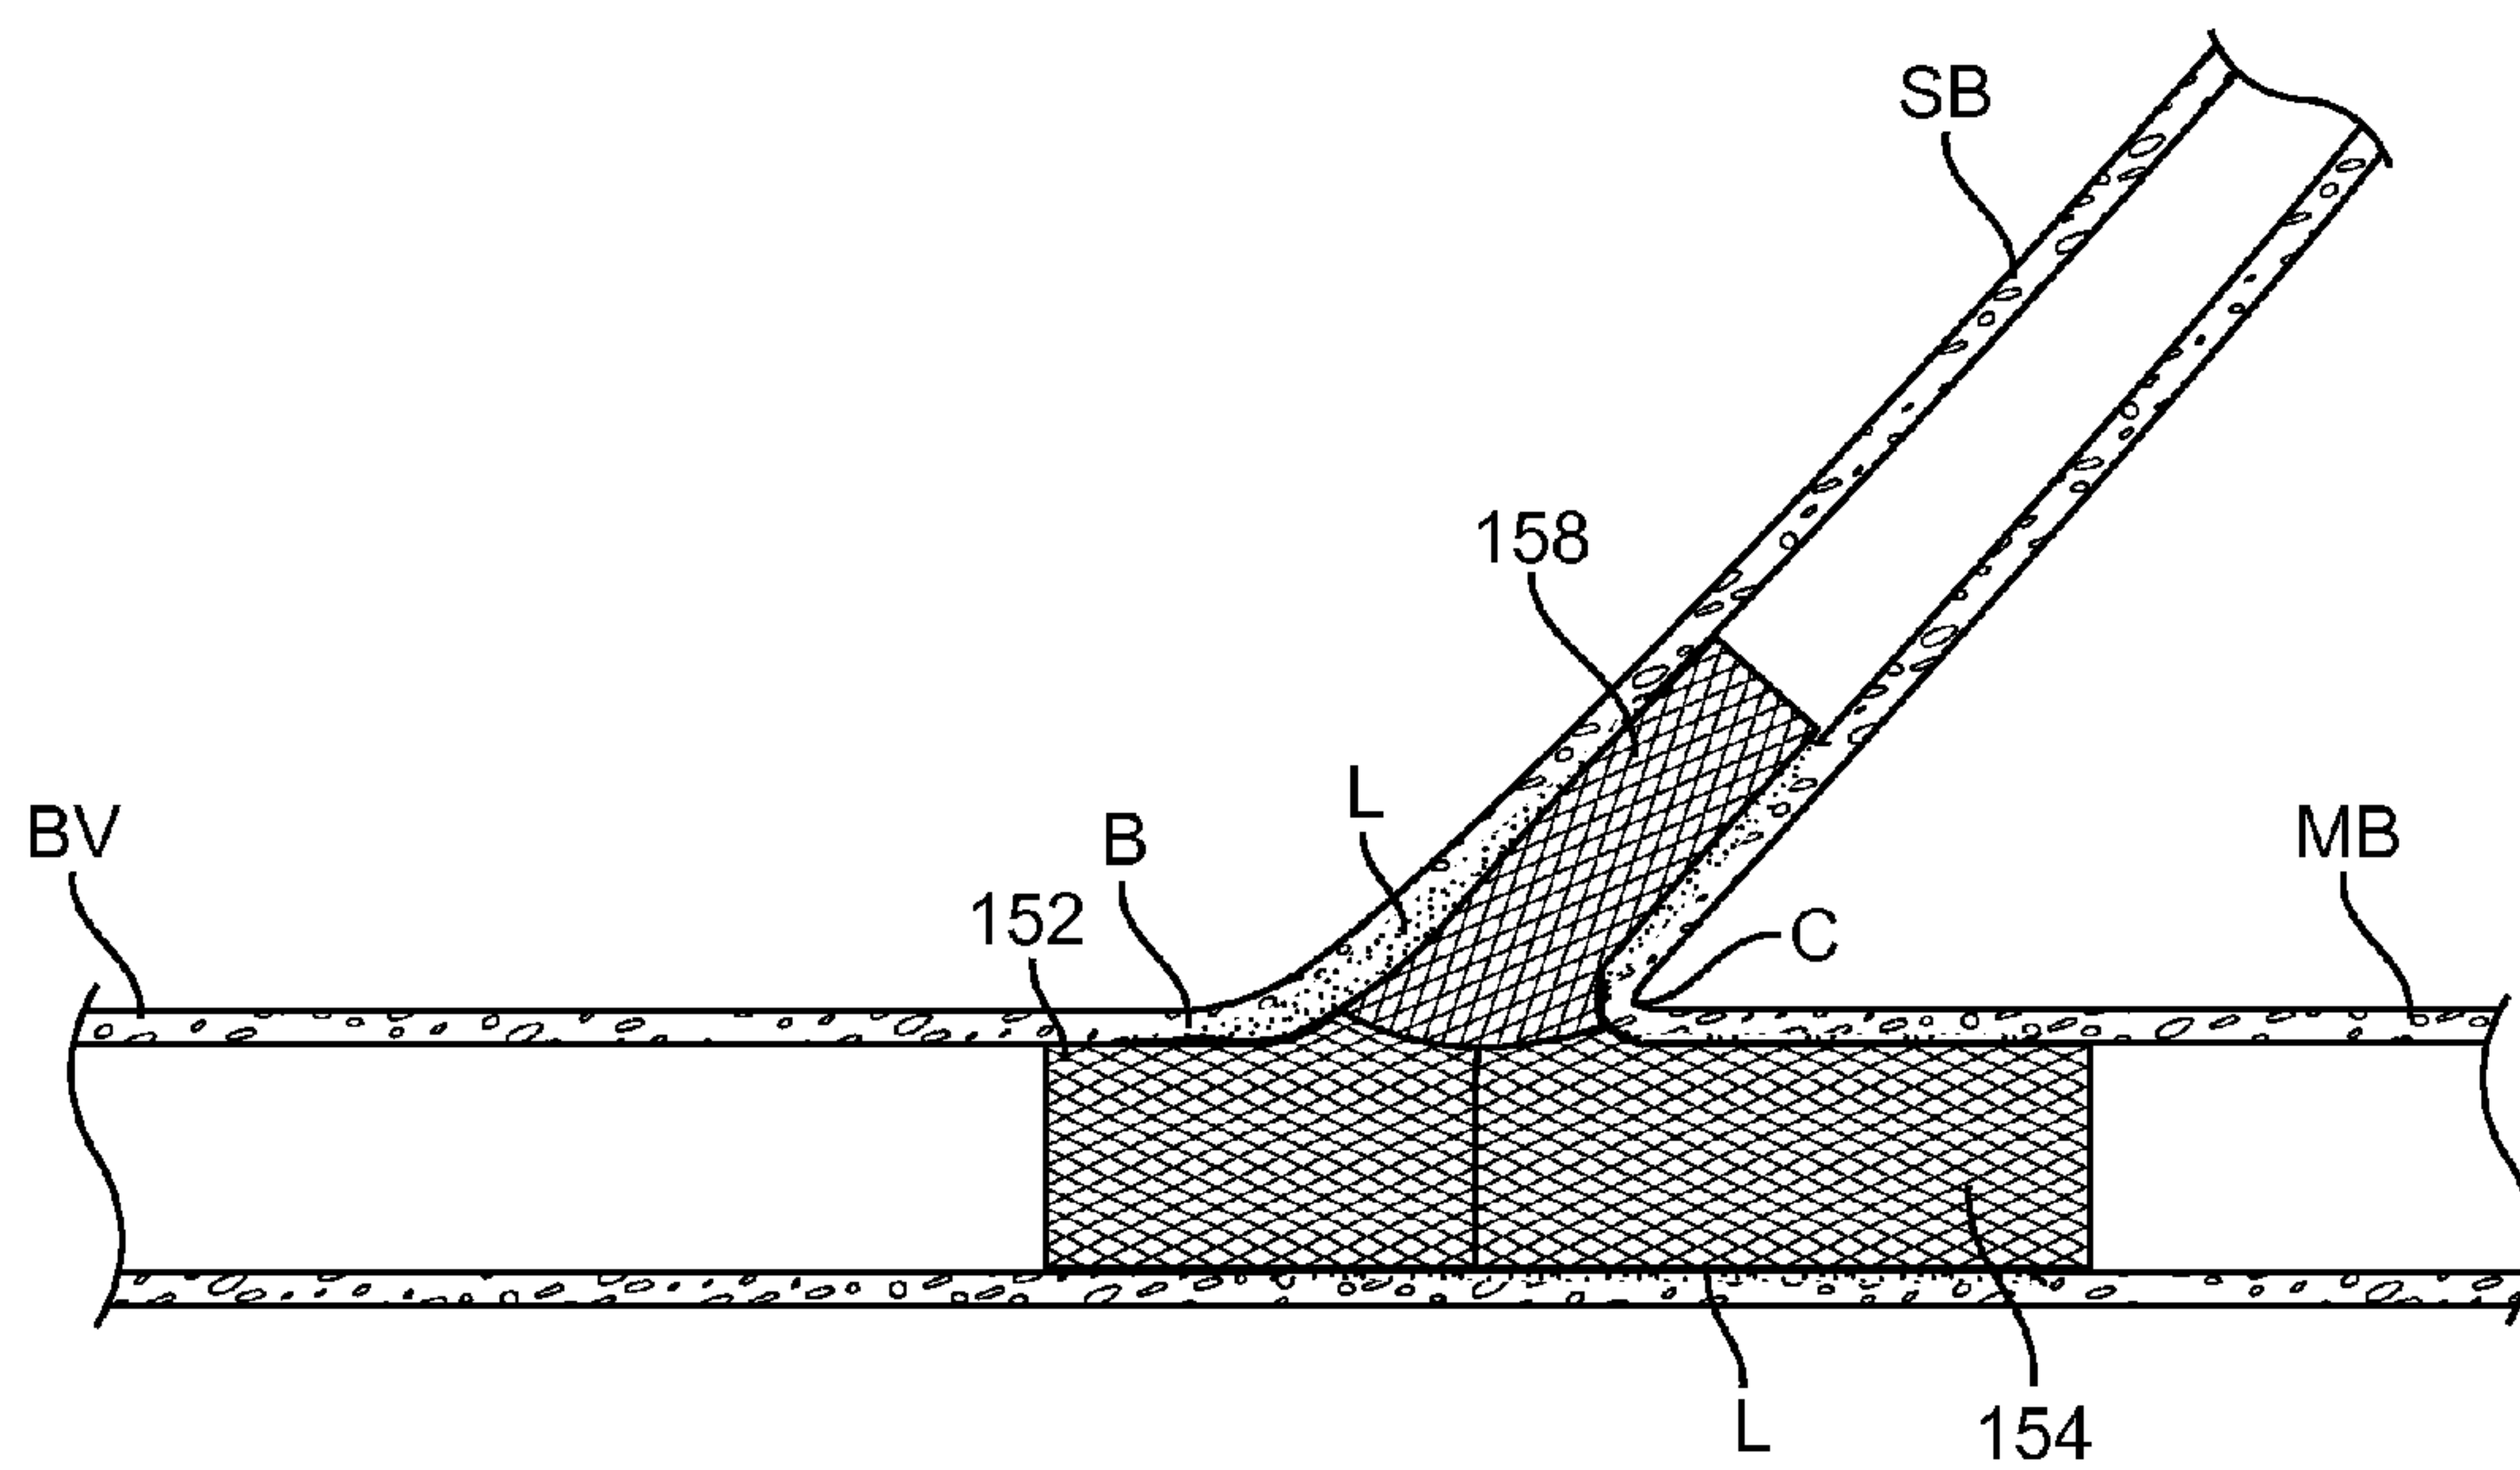


FIG. 6J

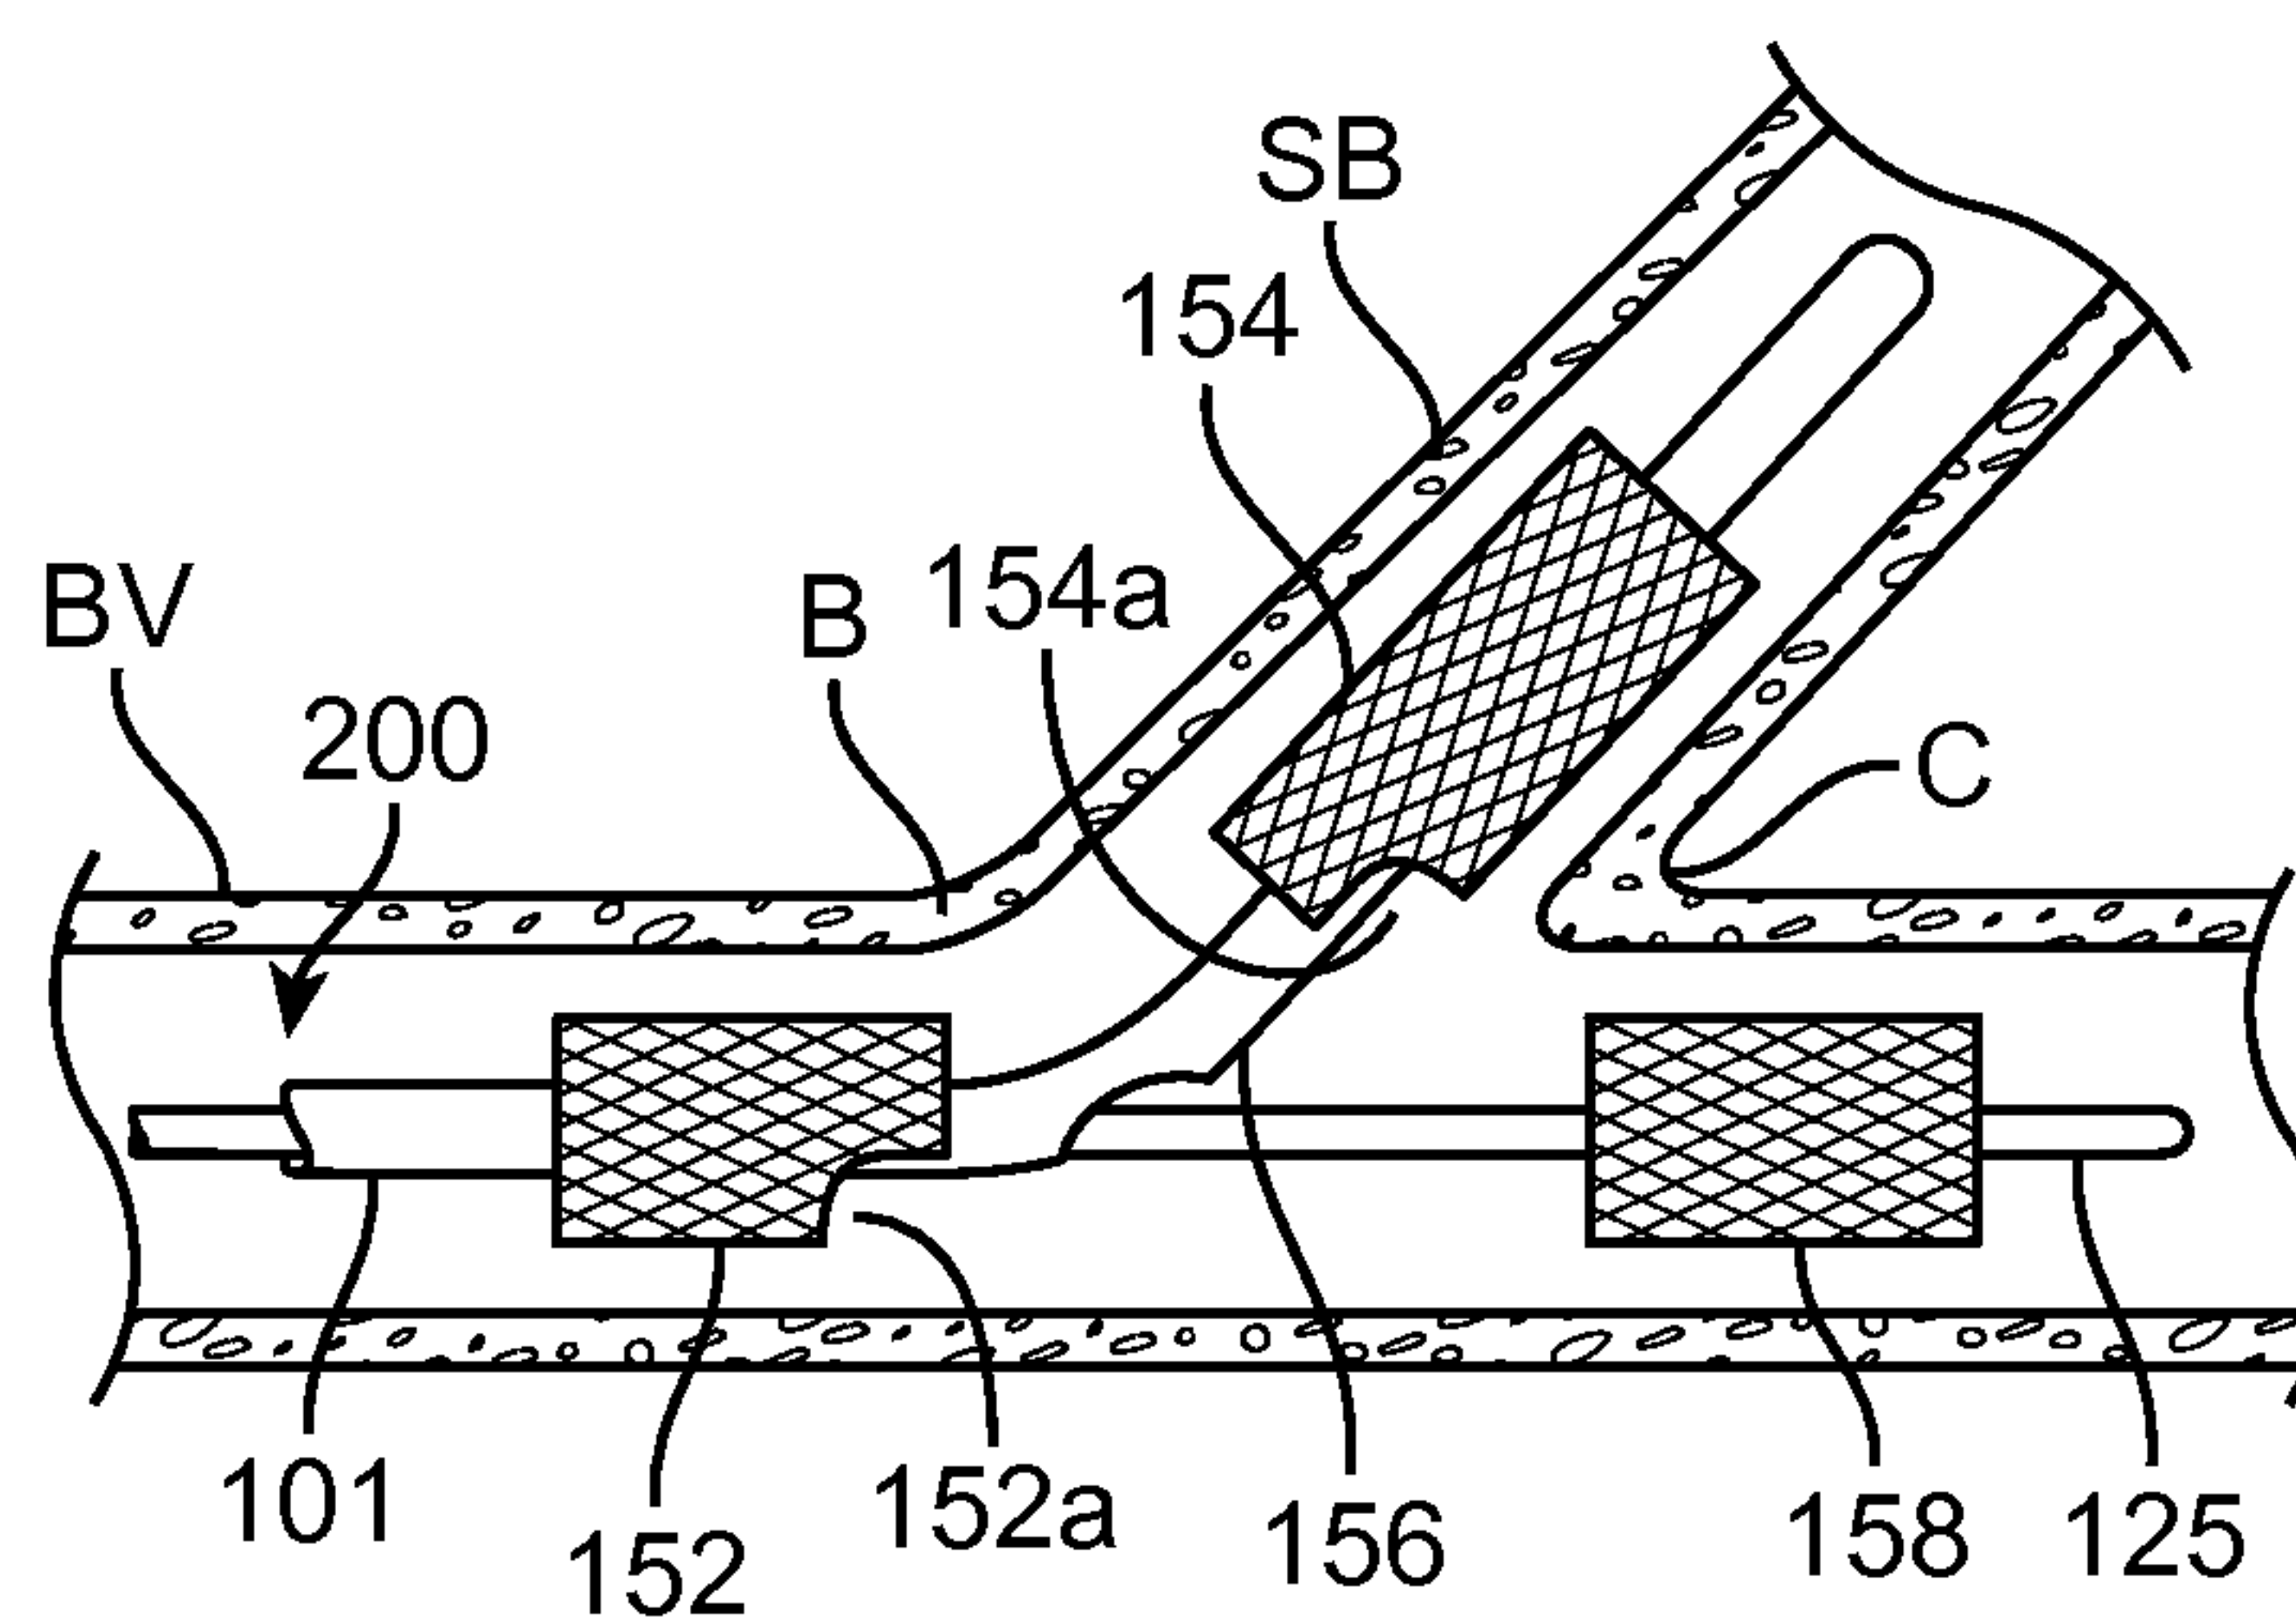


FIG. 7

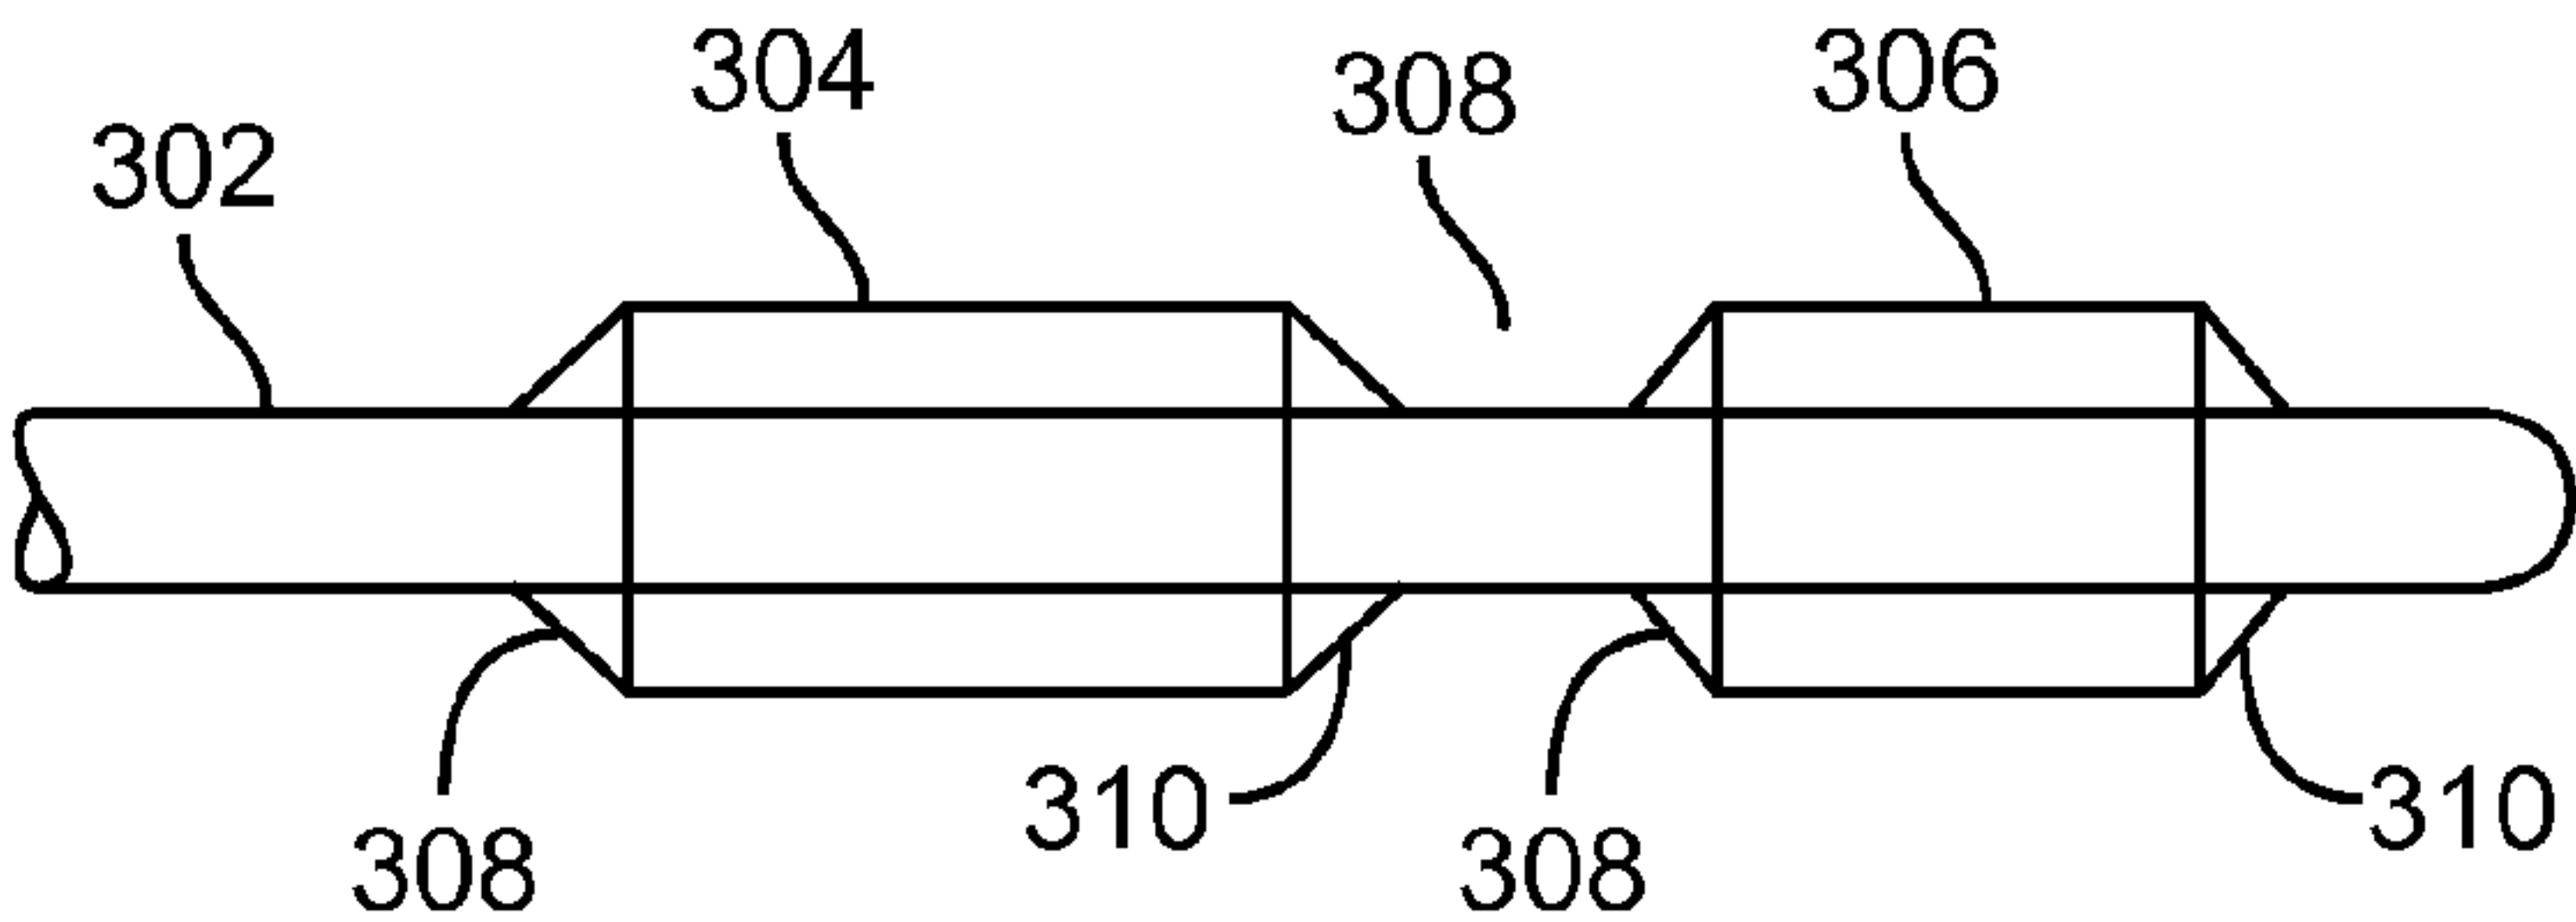


FIG. 8

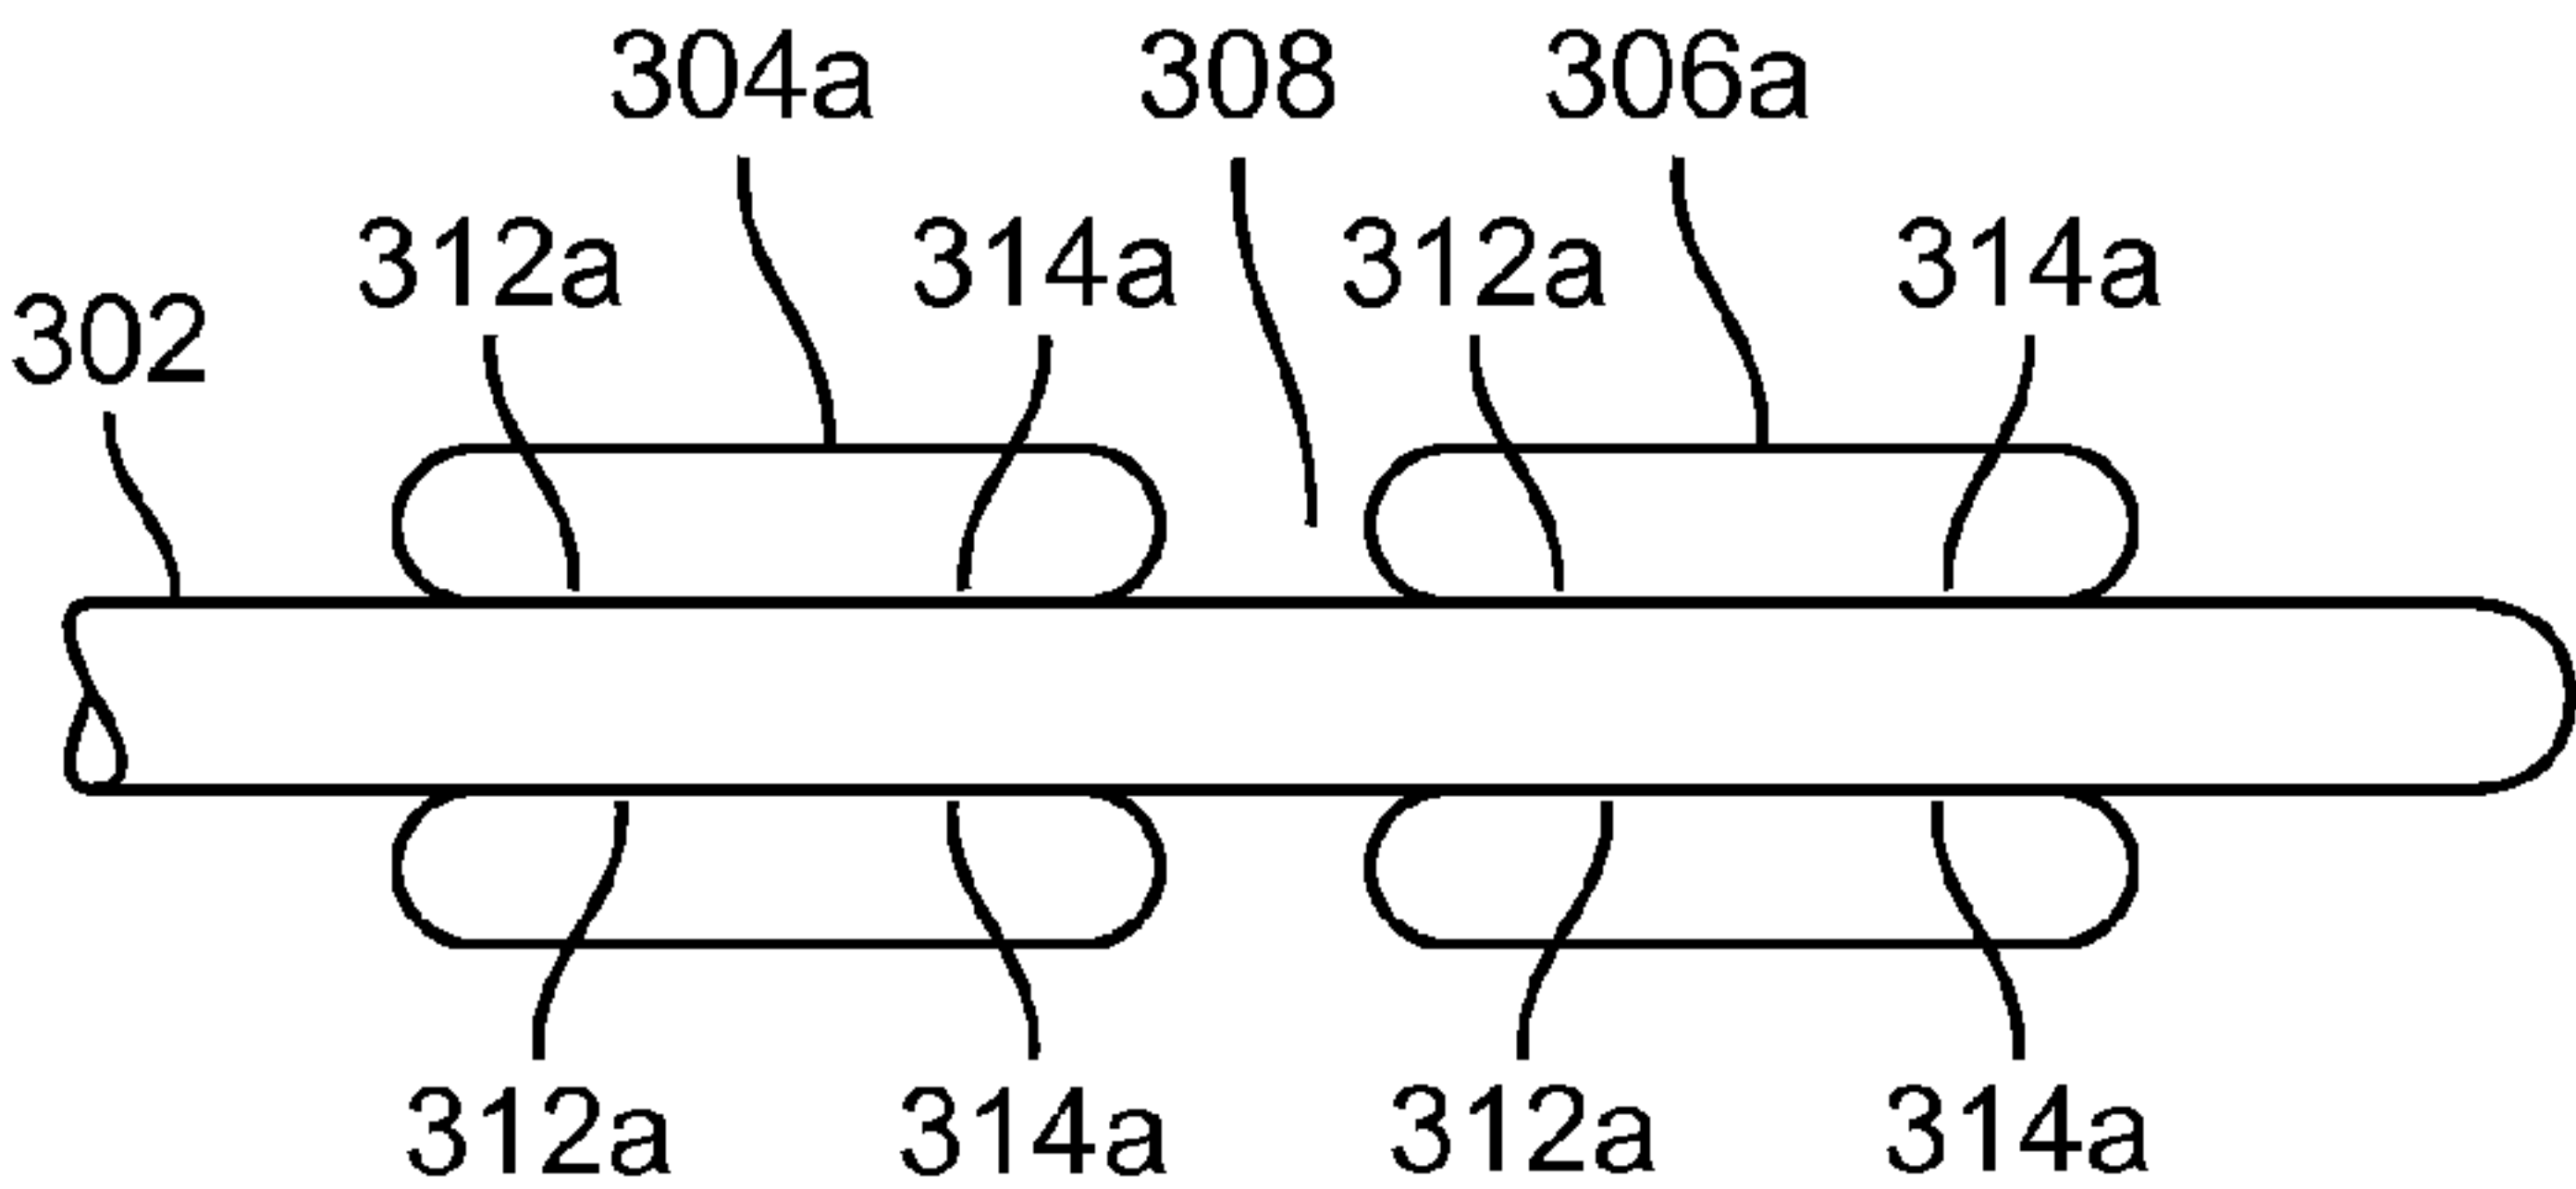


FIG. 9A

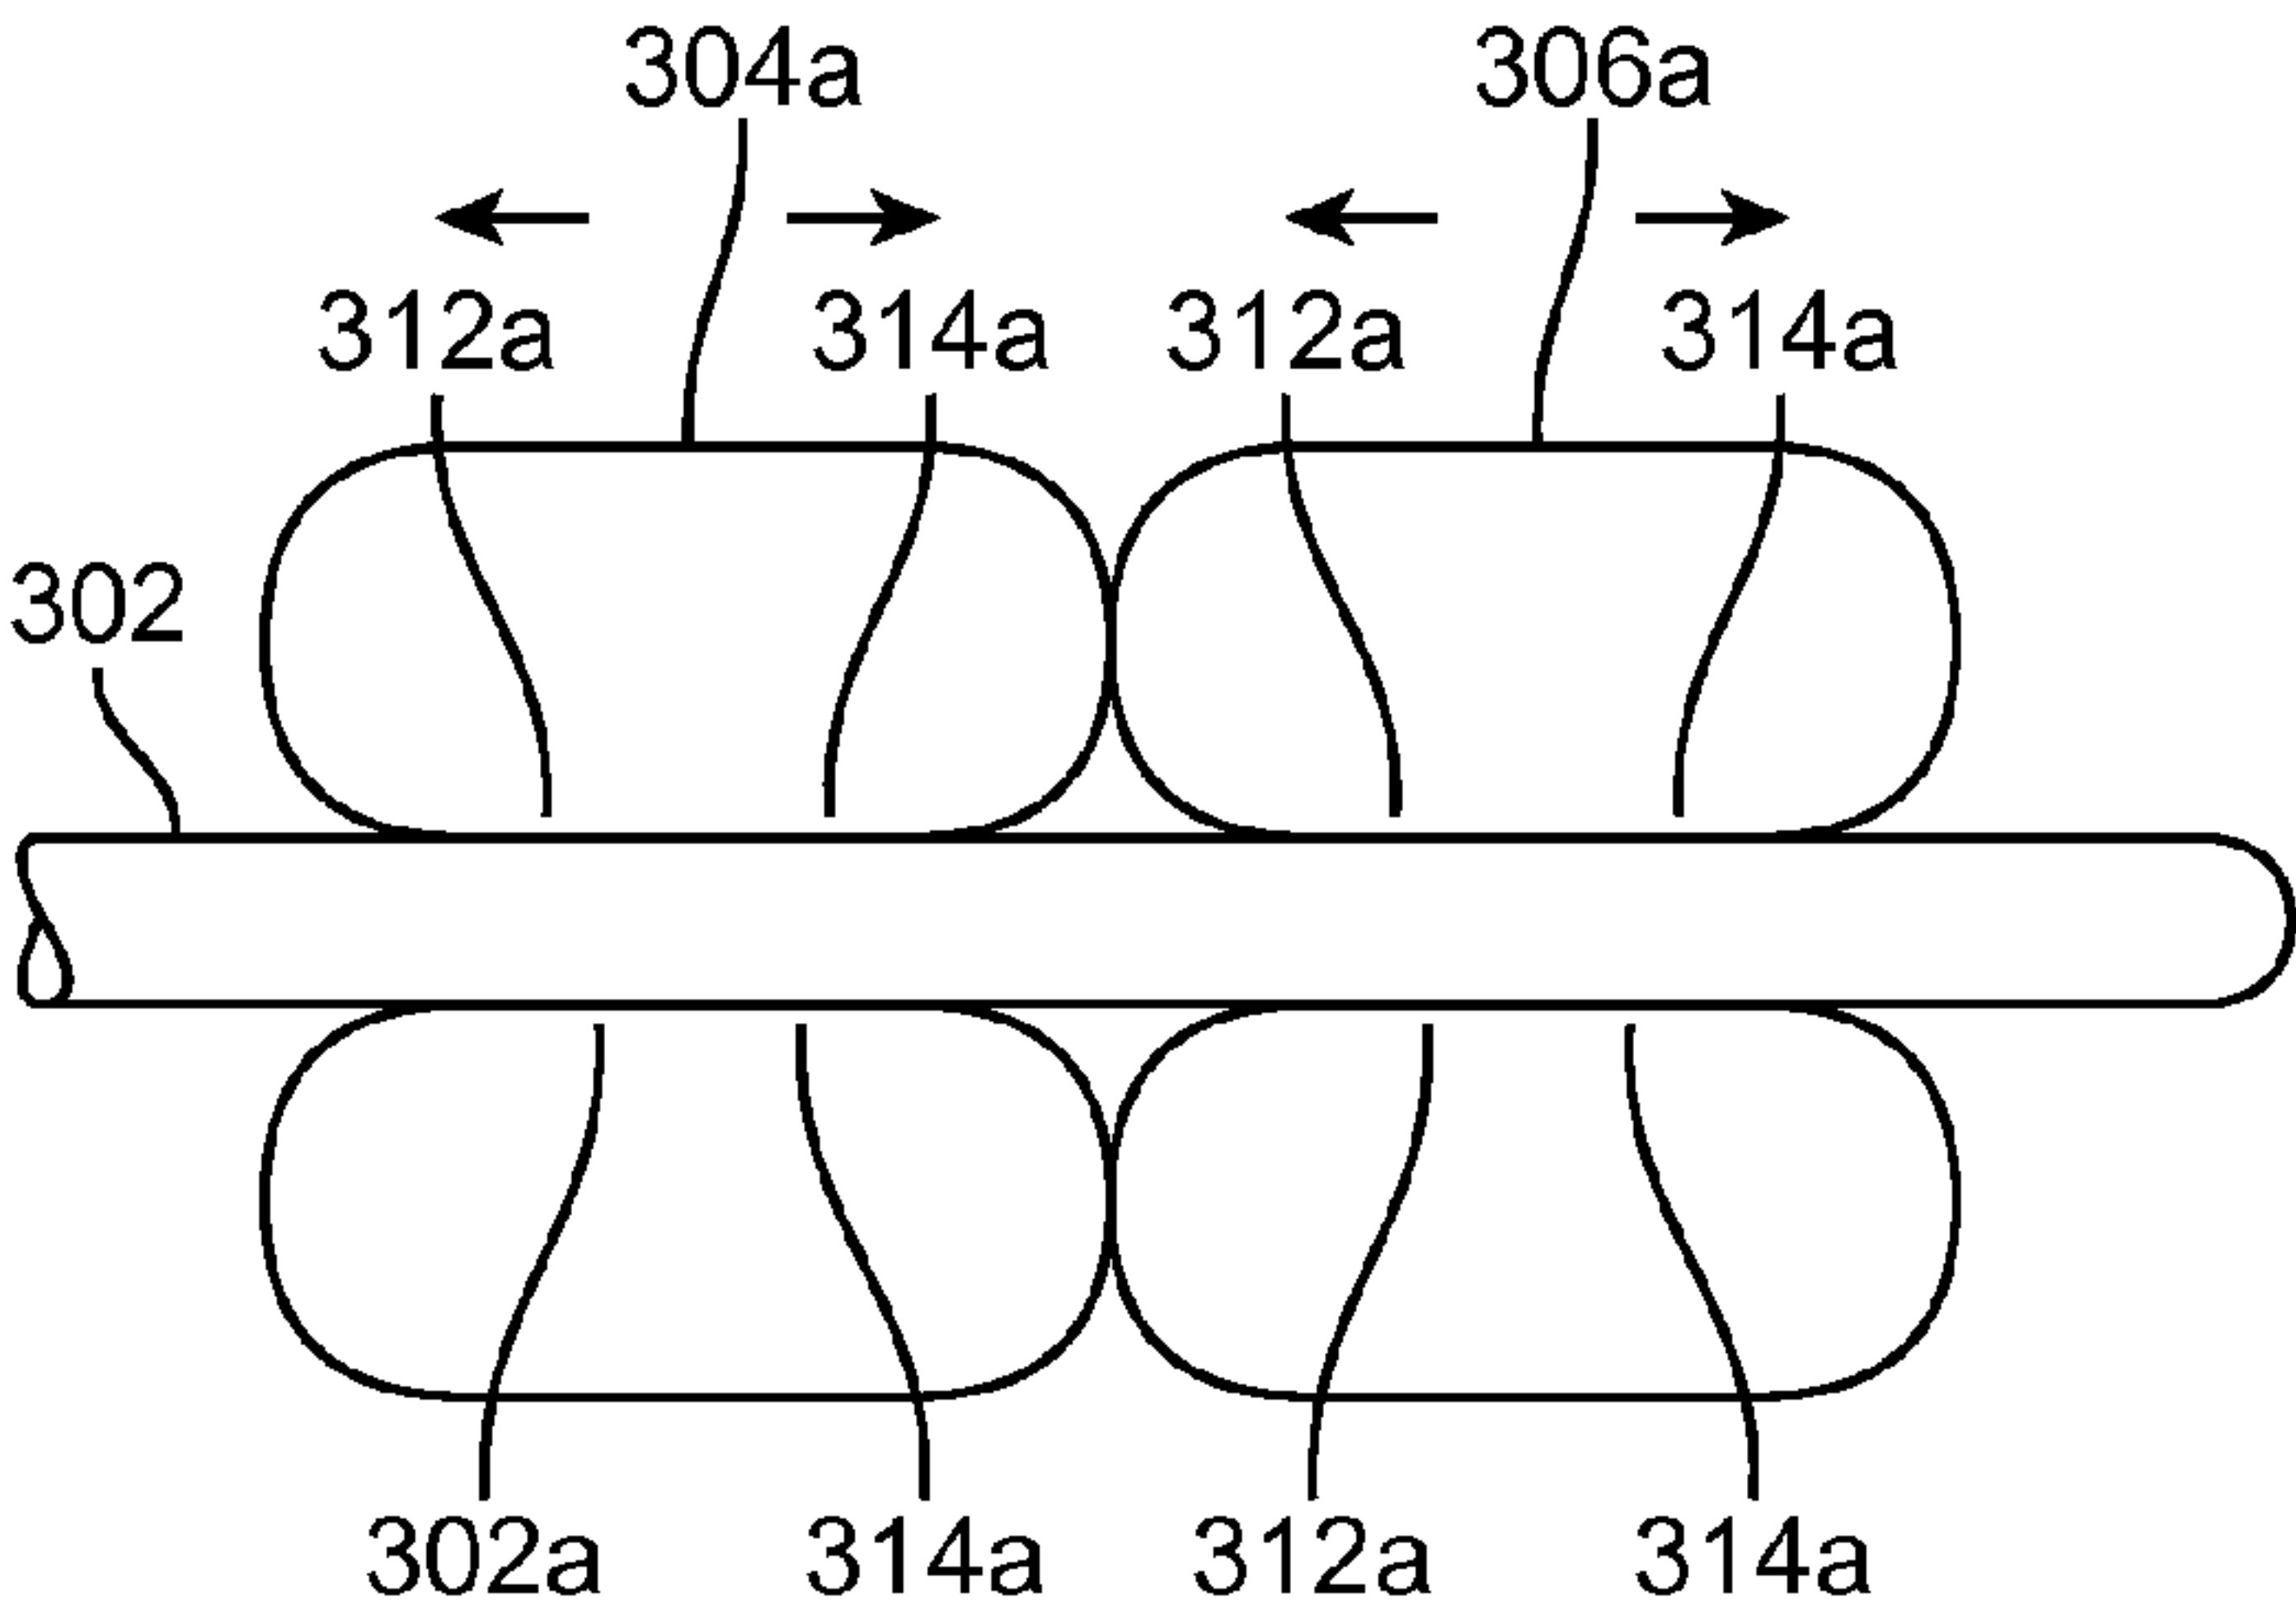


FIG. 9B

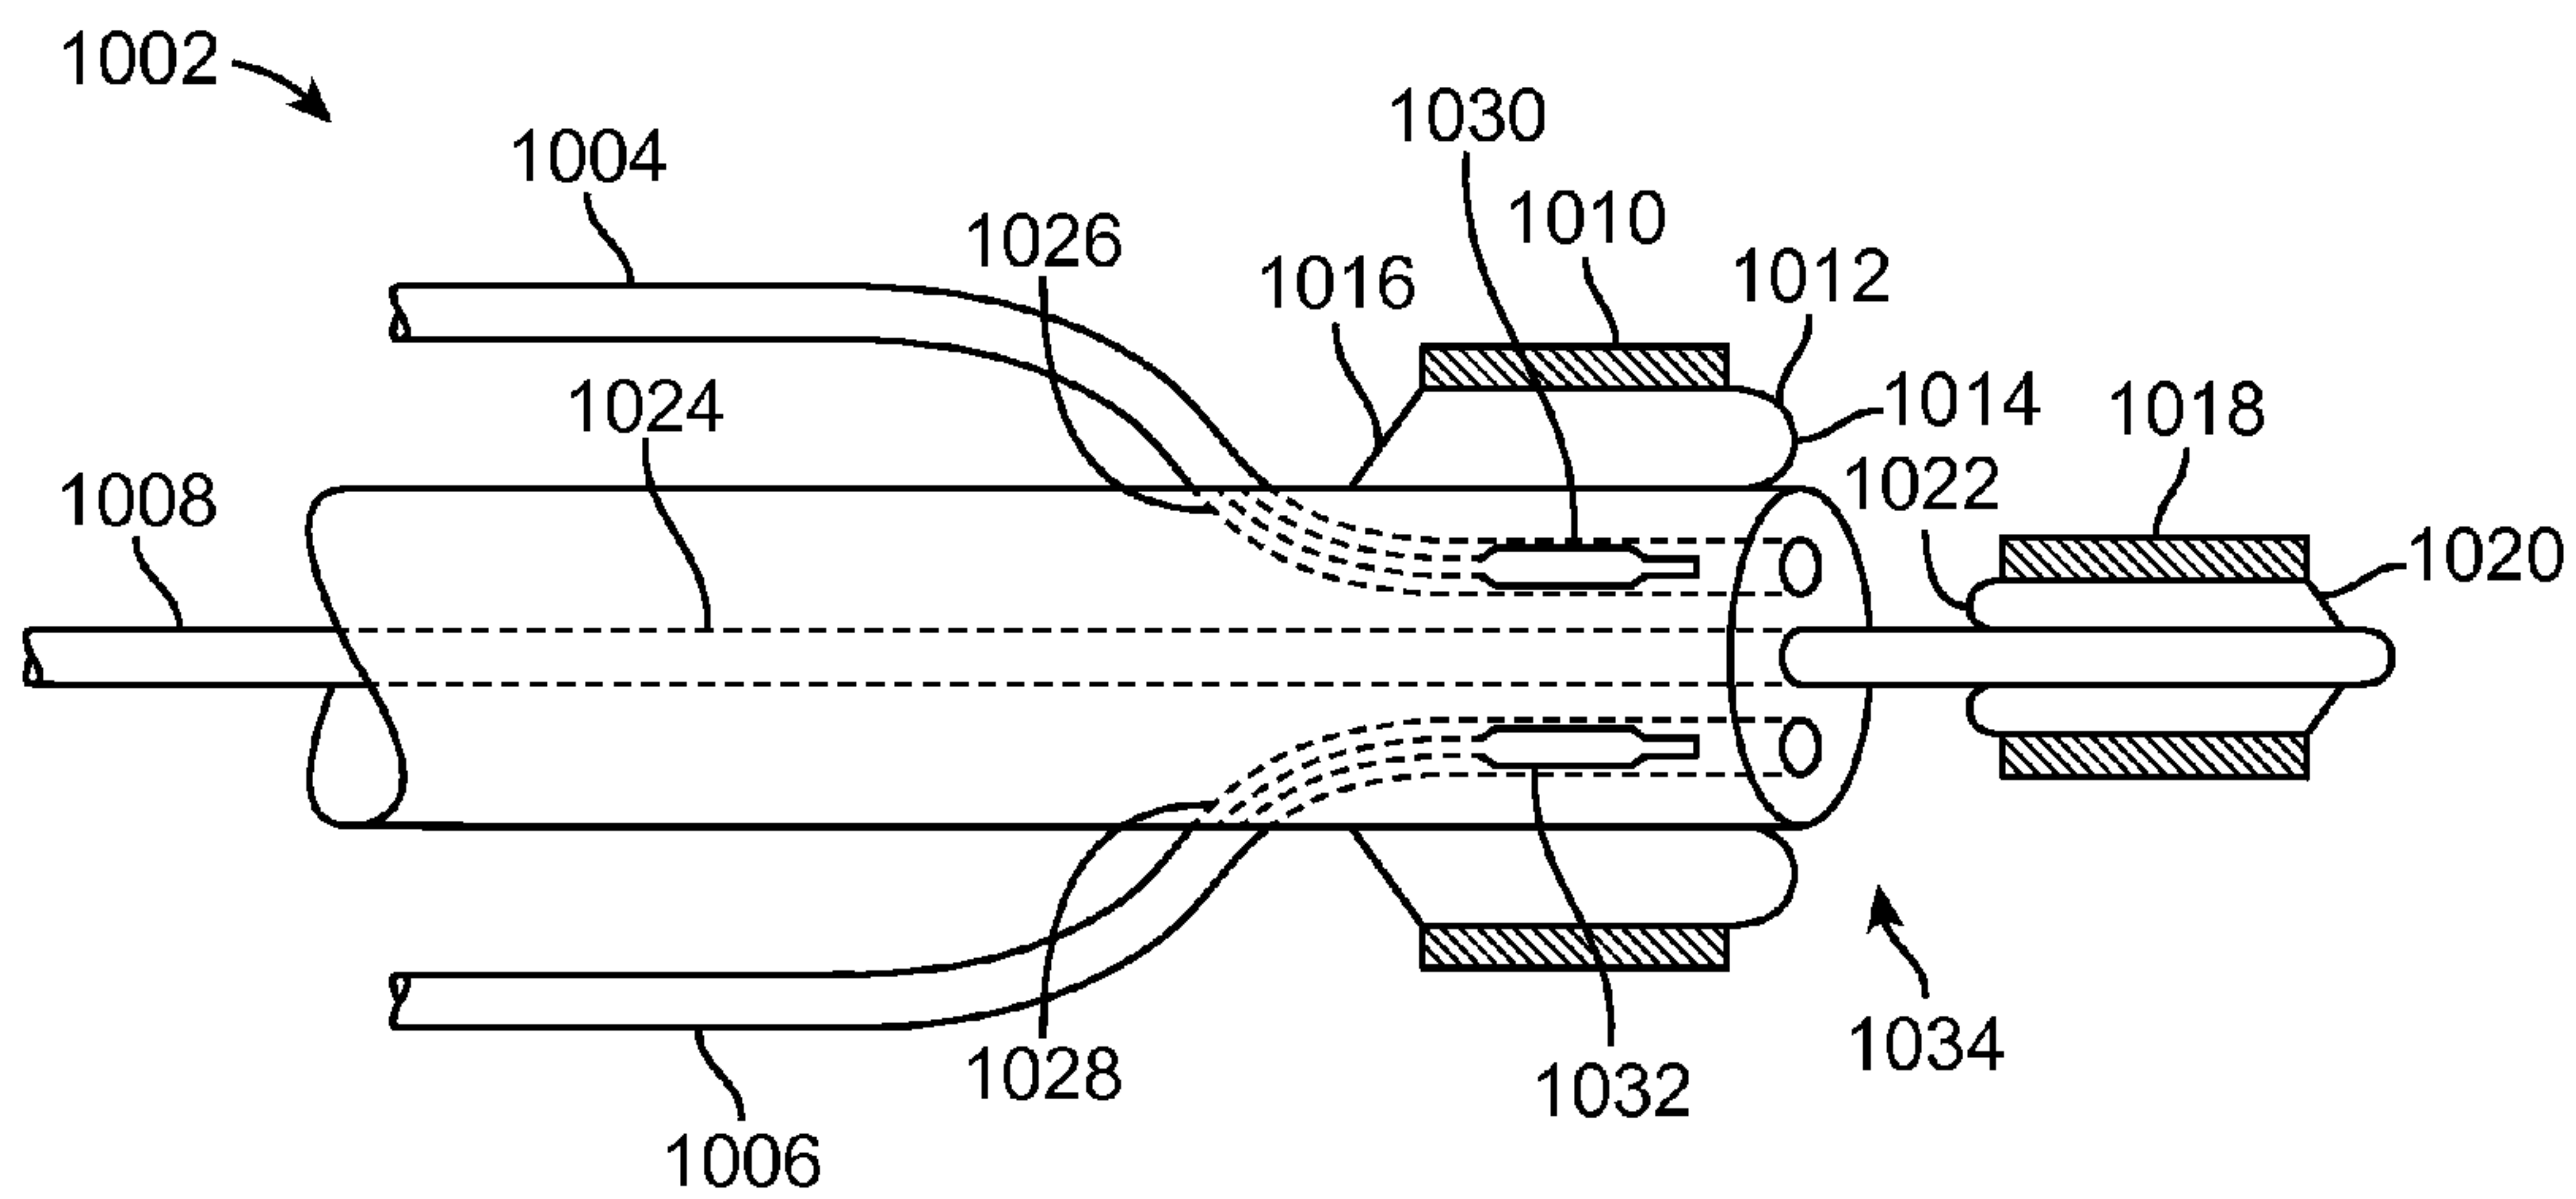


FIG. 10A

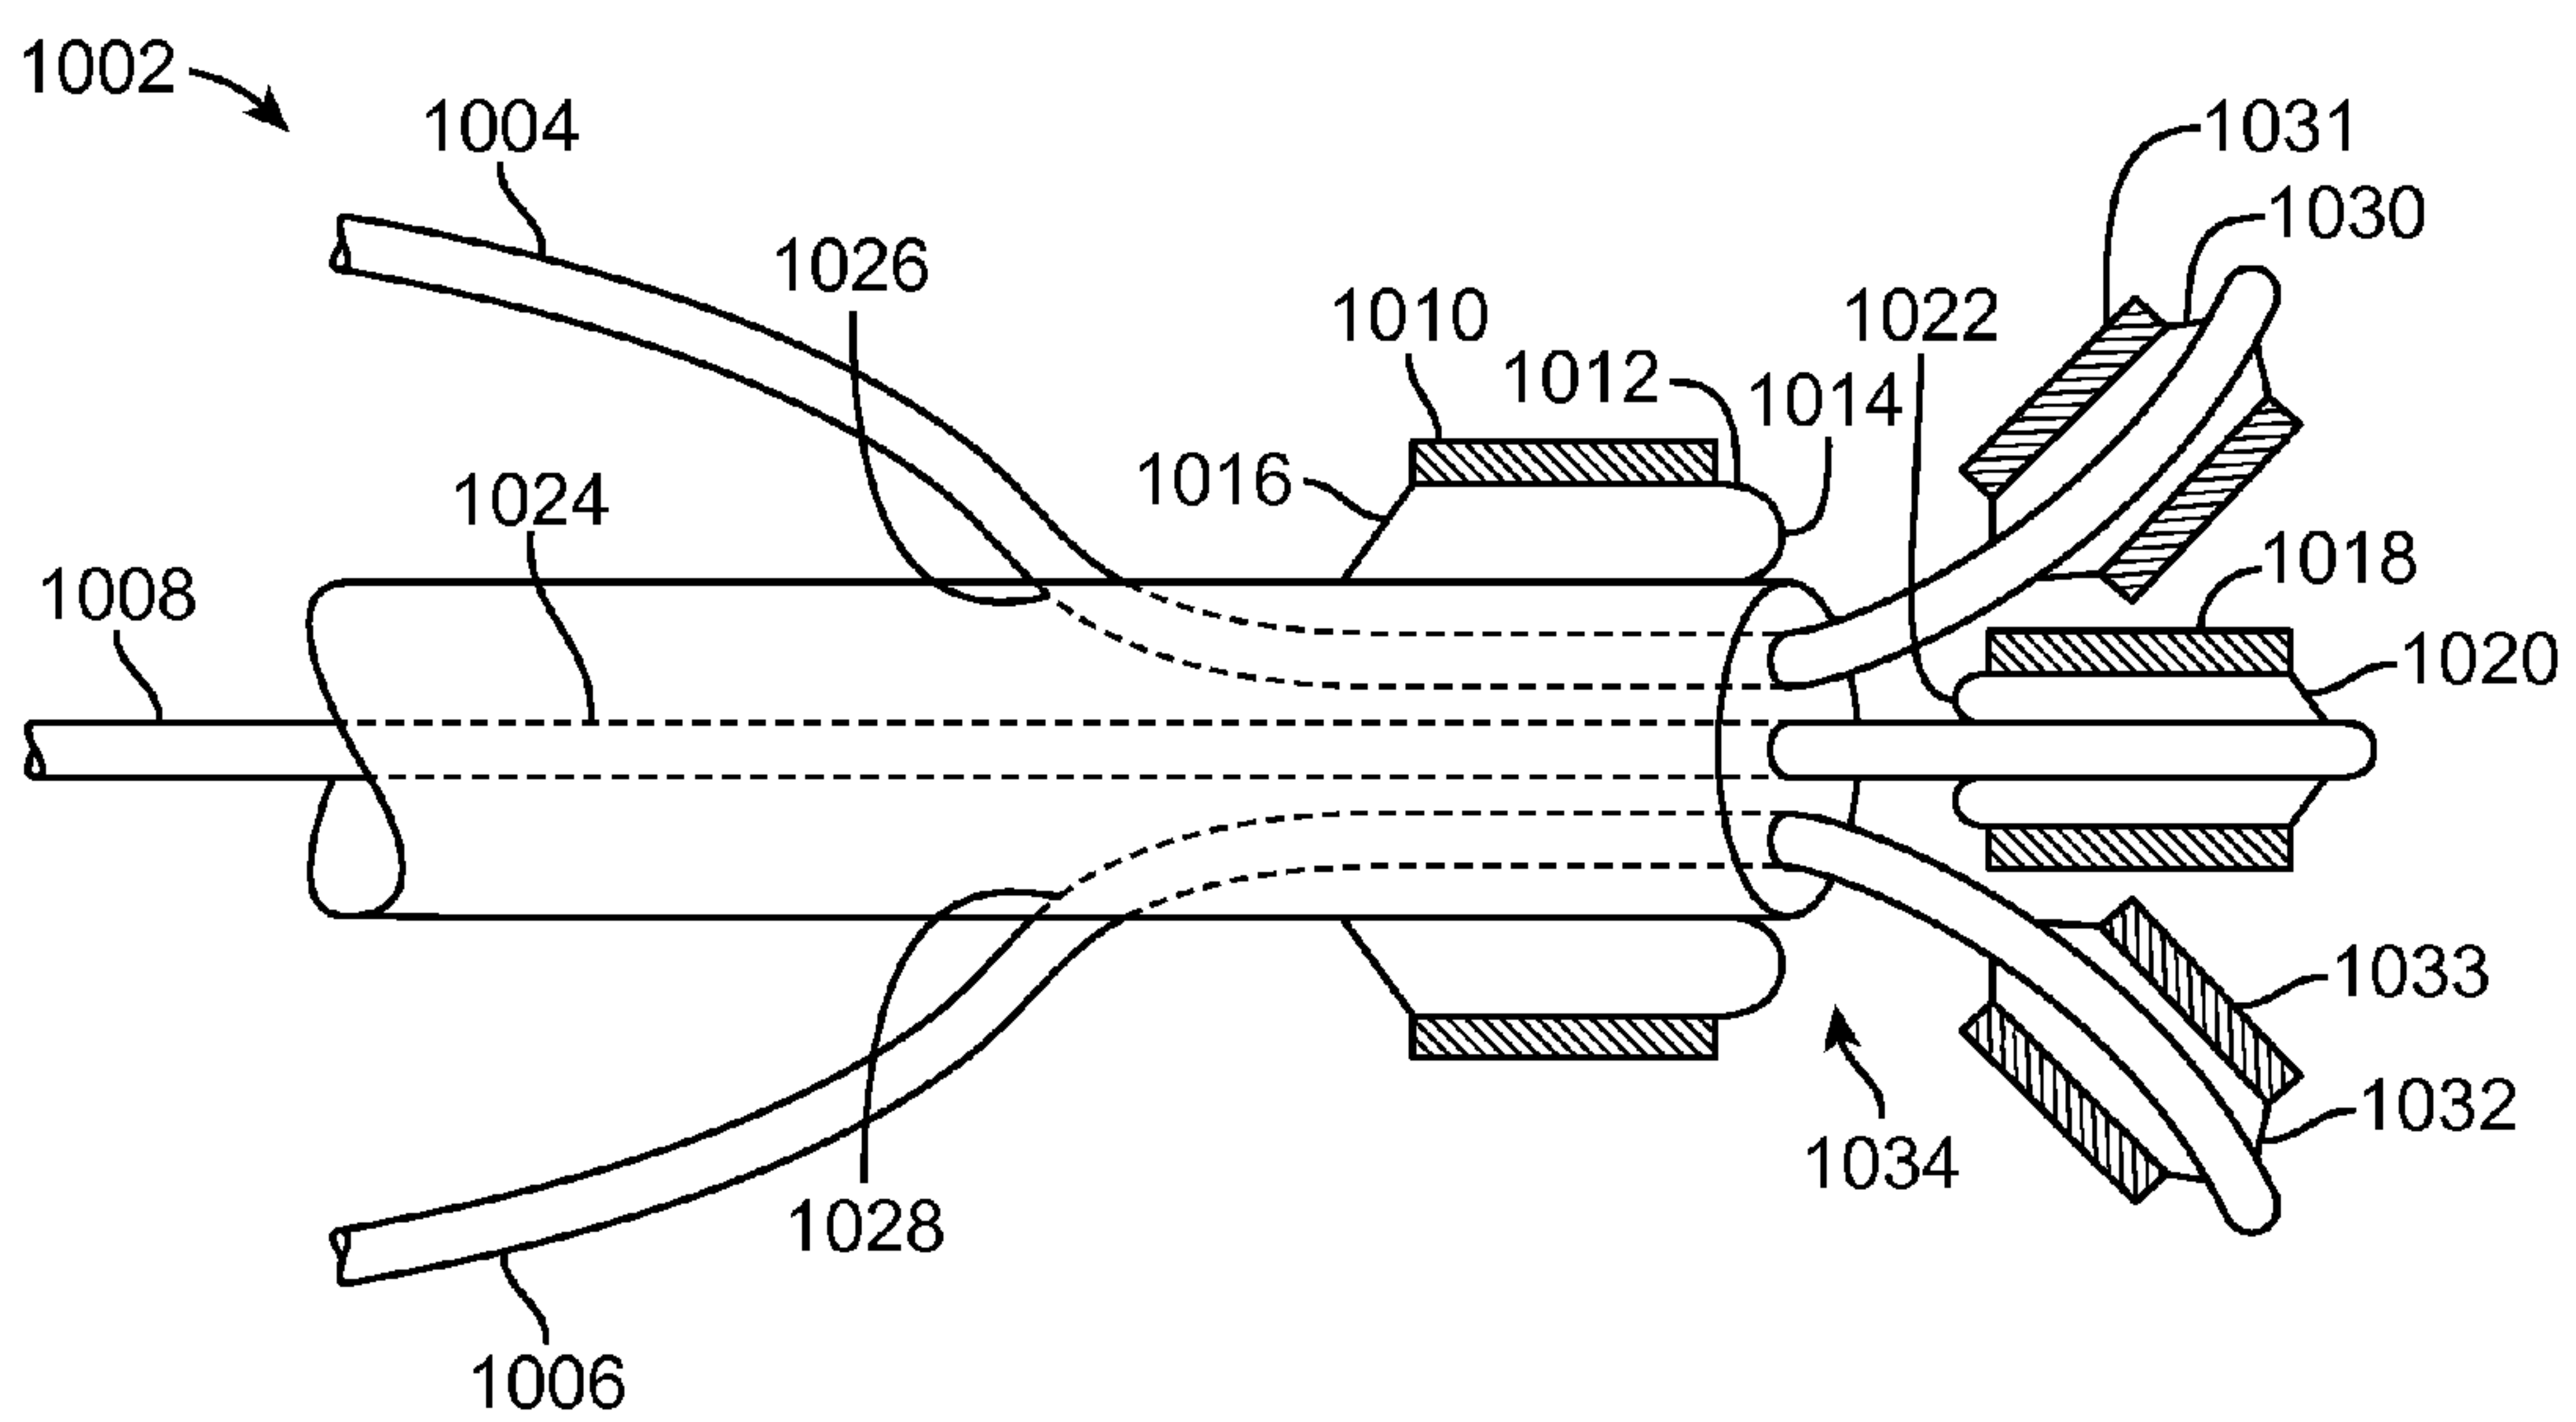


FIG. 10B

MULTI-STENT AND MULTI-BALLOON APPARATUS FOR TREATING BIFURCATIONS AND METHODS OF USE

CROSS REFERENCE TO RELATED APPLICATION DATA

The present application is a Continuation of PCT/US2012/024366 filed Feb. 8, 2012 (published as WO2012/109382 on Aug. 16, 2012), which application claims the benefit of U.S. Provisional Application No. 61/440,742 filed Feb. 8, 2011; the full disclosures, each of which are incorporated herein by reference in their entirety.

BACKGROUND OF THE INVENTION

Angioplasty and stenting of blood vessels or other body lumens are commonly performed today. Angioplasty is often performed by expanding a balloon in a vessel in order to reduce or eliminate plaque or other blockages. In many cases, a stent is also implanted in the vessel in order to further ensure a positive clinical result. A stent is an implantable scaffold that is typically delivered percutaneously and deployed in a vein, artery, or other tubular body organ for treating an occlusion, stenosis, aneurysm, collapse, dissection, or weakened, diseased, or abnormally dilated vessel or vessel wall. The stent is radially expanded in situ, thereby expanding and/or supporting the vessel wall or body organ wall. In particular, stents are quite commonly implanted in the coronary, cardiac, pulmonary, neurovascular, peripheral vascular, renal, gastrointestinal and reproductive systems. Stents have also been successfully used to reinforce other body parts, such as the urinary tract, the bile duct, the esophagus, the tracheo-bronchial tree and the brain.

Stents may improve angioplasty results by preventing elastic recoil and remodeling of the vessel wall. Stents also can be used to treat dissections in blood vessel walls that are caused by balloon angioplasty. In this situation, the stent is used to appose dissected intimal flaps of tissue which otherwise would extend into and block a vessel.

Conventional stents have also been used to treat more complex vascular problems, such as lesions at or near bifurcation points in the vascular system. A bifurcation is where a secondary artery (sometimes referred to as a side branch or daughter vessel) branches out of a typically larger vessel (sometimes referred to as the main branch or mother vessel). Stenting of bifurcations can present many challenges. For example, a stent that traverses the ostium of the side branch may obstruct blood flow into the side branch. Moreover, the struts in a stent may also block the side branch, limiting or preventing access to the side branch by another diagnostic or therapeutic device such as another catheter. This phenomenon is commonly referred to as "stent jailing." In still other situations, inflation of balloons and expansion of stents in a bifurcation can result in undesirable plaque shifting, which is sometimes referred to as "snow plowing." Other challenges with treatment of a bifurcated vessel can be the result of vessel spasm, dissection, thrombosis, etc.

More recently stents and balloons have also been used to elute drugs locally to the treatment site. Drugs such as rapamycin, everolimus, biolimus A9 and other analogs of rapamycin, as well as paclitaxel are promising in reducing restenosis rates, yet many of the aforementioned challenges of treating a bifurcation still exist.

It would therefore be desirable to provide improved medical devices and methods for treating bifurcated vessels. It would also be desirable to provide improved medical devices

and methods that are easier to use, safer, more reliable, and that provide a better clinical outcome compared with currently available medical devices.

Therefore, given the challenges of current stent technology, a need exists for improved stent delivery systems and methods, particularly for treating bifurcated vessels. At least some of these objectives will be met by the present invention.

BRIEF SUMMARY OF THE INVENTION

The present invention relates to methods and delivery systems used to dilate and/or deliver stents in a bifurcated vessel. Embodiments may be configured to stent at least a portion of a mother vessel and a portion of a daughter vessel.

In a first aspect of the present invention, a system for treating a patient's bifurcated vessel having a main branch and a side branch comprises a first delivery catheter and a second delivery catheter. The first delivery catheter carries a first stent which comprises a proximal stent and a distal stent. The first delivery catheter also has a first elongate shaft with a proximal and a distal end. A proximal expandable member has the proximal stent disposed thereover, and a distal expandable member has the distal stent disposed thereover. The proximal and distal expandable members are disposed adjacent the distal end of the first elongate shaft. The proximal and distal expandable members each have a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the collapsed configuration profile. The proximal and the distal expandable members are independently expandable of one another.

The second delivery catheter carries a second stent, and also has a second elongate shaft with a proximal and a distal end. A second expandable member with the second stent disposed thereover is disposed adjacent the distal end of the second elongate shaft. The second expandable member has a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the profile in the collapsed configuration. The second expandable member is independently expandable of the proximal and the distal expandable members.

In another aspect of the present invention, a system for dilating a bifurcated vessel having a main branch and a side branch in a patient comprises a first delivery catheter and a second delivery catheter. The first delivery catheter has a first elongate shaft with a proximal and a distal end, a proximal expandable member, and a distal expandable member. The proximal and distal expandable members are disposed adjacent the distal end of the first elongate shaft. The proximal and distal expandable members each have a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the collapsed configuration profile. The proximal and distal expandable members are independently expandable of one another.

The second delivery catheter has a second elongate shaft with a proximal and a distal end, and a second expandable member. The second expandable member is disposed adjacent the distal end of the second elongate shaft. The second expandable member has a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the profile

in the collapsed configuration. The second expandable member is independently expandable of the proximal and the distal expandable members.

The first delivery catheter may be adapted to deliver the proximal and distal stents to the main branch adjacent the bifurcation. The second delivery catheter may be adapted to deliver the second stent to the side branch adjacent the bifurcation. A portion of the second delivery catheter may be disposed under a portion of the proximal stent or under a portion of the distal stent, or under a portion of both. The second delivery catheter may be axially slidable relative to the first delivery catheter. The first elongate shaft may comprise a lumen which extends at least partially between proximal and distal ends of the first elongate shaft, and the lumen may be sized to slidably receive the second elongate shaft. The second delivery catheter may be fixed relative to the first delivery catheter so that relative axial movement between the two delivery catheters is prohibited.

Each of the stents may have a collapsed configuration suitable for delivery to the bifurcation, and a radially expanded configuration adapted to engage and support a vessel wall at the bifurcation or adjacent the bifurcation. Each of the stents may be crimped to its respective expandable member so as to prevent ejection of the stent during advancement through a patient's vasculature. A proximal end of the distal stent in the collapsed configuration may abut a distal end of the proximal stent in the collapsed configuration. A proximal end of the distal stent may abut a distal end of the proximal stent so as to form a sidehole in the first stent. The proximal end of the distal stent may comprise a notched region, and the distal end of the proximal stent may also comprise a notched region. The second delivery catheter may slidably pass through the side hole in the first stent. A proximal end of the second stent may comprise a beveled section adapted to fit flush against a sidewall of the proximal stent or a sidewall of the distal stent. A proximal end of the second stent in the radially expanded configuration may be aligned with and abut a side of both the proximal stent in the radially expanded configuration and a side of the distal stent in the radially expanded configuration.

A gap may separate the proximal and the distal expandable members when both the proximal and the distal expandable members are in the collapsed configuration. The gap may be disposed between a proximal end of distal expandable member and a distal end of the proximal expandable member. Expansion of the proximal and the distal members may displace the proximal end of the distal expandable member relative to the distal end of the proximal expandable member so that the proximal end of the distal expandable member advances toward the distal end of the proximal expandable member. This may decrease the gap between the proximal and the distal expandable members. The proximal end of the distal expandable member may abut the distal end of the proximal expandable member when both the proximal and the distal expandable members are in the expanded configuration. The proximal expandable member, the distal expandable member, or the second expandable member may comprise a balloon. A proximal end of the second expandable member may abut a side of both the proximal and the distal expandable members when the proximal, the distal, and the second expandable members are in the radially expanded configuration.

At least one of the first elongate shaft or the second elongate shaft may comprise a guidewire lumen extending at least partially between its proximal and distal ends. The guidewire lumen may be sized to slidably receive a guidewire. The first elongate shaft may comprise a proximal guidewire port and a

distal guidewire port adjacent the distal end thereof, and the proximal guidewire port may be closer to the proximal end of the first elongate shaft than the distal end of the first elongate shaft. The proximal guidewire port may be closer to the distal guidewire port than the proximal end of the first elongate shaft. The second elongate shaft may comprise a proximal guidewire port and a distal guidewire port adjacent the distal end thereof, and the proximal guidewire port may be closer to the proximal end of the second elongate shaft than the distal end of the second elongate shaft. The proximal guidewire port may be closer to the distal guidewire port than the proximal end of the second elongate shaft.

In still another aspect of the present invention, a method for treating a bifurcated vessel having a main branch and a side branch in patient comprises providing a first delivery catheter and a second delivery catheter. The first delivery catheter comprises a proximal expandable member, a distal expandable member and a first stent. The proximal and distal expandable members are disposed near a distal end of the first delivery catheter. The first stent comprises a proximal stent and a distal stent. The proximal stent is disposed over the proximal expandable member, and the distal stent is disposed over the distal expandable member. A distal portion of the proximal stent comprises a notched region, and a proximal portion of the distal stent comprises a notched region. The two notched regions are adjacent one another to form a side hole in the first stent.

The second delivery catheter comprises a second expandable member and a second stent. The second expandable member is disposed near a distal end of the second delivery catheter, and the second stent is disposed over the second expandable member. The second delivery catheter passes through the side hole in the first stent. Advancing the first and the second delivery catheter positions the two catheters toward the bifurcation so that the side hole in the first stent may be aligned with the side branch. The second stent is radially expanded from a collapsed configuration to an expanded configuration. The proximal stent is radially expanded from a collapsed configuration to an expanded configuration, and the distal stent is radially expanded from a collapsed configuration to an expanded configuration.

Advancing the first and the second delivery catheters may comprise advancing the first delivery catheter or the second delivery catheter over a guidewire. Aligning the side hole may comprise advancing the first delivery catheter and the second delivery catheter until one or more of the delivery catheters engage a carina of the bifurcation.

Radially expanding the second stent may comprise expanding the second stent to engage a wall of the side branch or a wall of the main branch. Radially expanding the second stent may also comprise expanding the second expandable member. The second expandable member may comprise a balloon, and expanding the second expandable member may comprise inflating the balloon. The second stent may be radially expanded prior to radial expansion of the proximal stent or the distal stent.

Radially expanding the proximal stent may comprise expanding the proximal stent to engage a wall of the main branch. Radially expanding the proximal stent may also comprise expanding the proximal expandable member. The proximal expandable member may comprise a balloon, and expanding the proximal expandable member may comprise inflating the balloon. The proximal stent may be radially expanded before radial expansion of the distal stent.

Radially expanding the distal stent may comprise expanding the distal stent to engage a wall of the main branch or a wall of the side branch. Radially expanding the distal stent

5

may also comprise expanding the distal expandable member. The distal expandable member may comprise a balloon, and expanding the distal expandable member may comprise inflating the balloon.

The method may further comprise proximally retracting the second delivery catheter so that a proximal end of the second stent is aligned with the side hole in the first stent. A proximal end of the second stent may be aligned with an ostium of the side branch. Proximally retracting the second delivery catheter may comprise aligning a radiopaque marker on the second delivery catheter with a radiopaque marker on the first delivery catheter. Proximally retracting the second delivery catheter may comprise sliding the second delivery catheter under a portion of the first stent. The second delivery catheter may slide under a portion of the proximal stent or under a portion of the distal stent. Proximally retracting the second delivery catheter may comprise sliding the second delivery catheter through the side hole in the first stent. A proximal portion of the second stent may abut both a distal portion of the proximal stent and a proximal portion of the distal stent after radial expansion of the proximal stent, the distal stent, and the second stent. The distal portion of the proximal stent may abut the proximal portion of the distal stent after radial expansion of the stents.

In still another aspect of the present invention, a method for treating a bifurcated vessel having a main branch and a side branch in a patient comprises providing a first delivery catheter and a second delivery catheter. The first delivery catheter comprises a proximal expandable member, a distal expandable member and a first stent. The proximal and distal expandable members are disposed near a distal end of the first delivery catheter. The first stent comprises a proximal stent and a distal stent. The proximal stent is disposed over the proximal expandable member, and the distal stent is disposed over the distal expandable member. A distal portion of the proximal stent comprises a notched region, and a proximal portion of the distal stent comprises a notched region. The notched regions are adjacent one another to form a side hole in the first stent.

The second delivery catheter comprises a second expandable member and a second stent. The second expandable member is disposed near a distal end of the second delivery catheter, and the second stent is disposed over the second expandable member. The second delivery catheter passes through the side hole in the first stent. Advancing the first and second delivery catheters positions them toward the bifurcation. The first stent and the second stent are positioned at the bifurcation such that the proximal stent is disposed in the main branch, the distal stent is disposed in the side branch, and the second stent is disposed in the main branch downstream of the bifurcation. The side hole in the first stent is aligned with the main branch and faces downstream of the bifurcation. The distal stent is radially expanded from a collapsed configuration to an expanded configuration. The proximal stent is radially expanded from a collapsed configuration to an expanded configuration. The second stent is radially expanded from a collapsed configuration to an expanded configuration.

In yet another aspect of the present invention, a method for treating a bifurcated vessel having a main branch and a side branch in a patient comprises providing a first delivery catheter and a second delivery catheter. The first delivery catheter comprises a proximal expandable member and a distal expandable member. The proximal and distal expandable members are disposed near a distal end of the first delivery catheter, and the expandable members are independently expandable from one another. The second delivery catheter

6

comprises a second expandable member disposed near a distal end thereof. The first and second delivery catheters are advanced toward the bifurcation and the second expandable member is positioned in the side branch. The proximal and distal expandable members are positioned in the main branch so that the proximal expandable member is at least partially upstream of the bifurcation, and the distal expandable member is at least partially downstream of the bifurcation. The second expandable member is radially expanded from a collapsed configuration to an expanded configuration. The proximal expandable member is radially expanded from a collapsed configuration to an expanded configuration. The distal expandable member is radially expanded from a collapsed configuration to an expanded configuration.

Radially expanding the second expandable member may comprise expanding the second expandable member into engagement with a wall of the side branch or the main branch. The second expandable member may comprise a balloon, and expanding the second expandable member may comprise inflating the balloon. The second expandable member may be expanded prior to radial expansion of the proximal expandable member or the distal expandable member.

Radially expanding the proximal expandable member may comprise expanding the proximal expandable member to engage a wall of the main branch. The proximal expandable member may comprise a balloon, and expanding the expandable member may comprise inflating the balloon. The proximal expandable member may be expanded before radial expansion of the distal expandable member, or before expansion of the second expandable member. The proximal expandable member may also be expanded simultaneously with the distal expandable member, the second expandable member, or simultaneously with both.

Radially expanding the distal expandable member may comprise expanding the distal expandable member to engage a wall of the main branch or the side branch. The distal expandable member may comprise a balloon, and expanding the distal expandable member may comprise inflating the balloon. The distal expandable member may be expanded before expansion of the proximal expandable member or second expandable member.

The method may further comprise proximally retracting the second delivery catheter so that a proximal end of the second expandable member is aligned with an ostium of the side branch. Proximally retracting the second delivery catheter may comprise sliding the second delivery catheter under a portion of the proximal expandable member. Both the proximal and distal expandable members may be radially expanded simultaneously. A proximal portion of the distal expandable member may engage a distal portion of the proximal expandable member.

In still another aspect of the present invention, a method for treating a bifurcated vessel having a main branch and a side branch in a patient comprises providing a first delivery catheter and a second delivery catheter. The first delivery catheter comprises a proximal expandable member and a distal expandable member. The proximal and distal expandable members are disposed near a distal end of the first delivery catheter. The proximal and the distal expandable members are independently expandable from one another. The second delivery catheter comprises a second expandable member disposed near a distal end thereof. The first and second delivery catheters are advanced toward the bifurcation, and the proximal expandable member is positioned in the main branch adjacent the bifurcation. The distal expandable member is positioned in the side branch adjacent the bifurcation. The second expandable member is positioned in the main

branch downstream of the proximal expandable member. The distal expandable member is radially expanded from a collapsed configuration to an expanded configuration. The proximal expandable member is radially expanded from a collapsed configuration to an expanded configuration. The second expandable member is radially expanded from a collapsed configuration to an expanded configuration.

In yet another aspect of the present invention, a system for treating a patient with a trifurcated vessel having a main branch, a first side branch, and a second side branch comprises a first delivery catheter, a second delivery catheter and a third delivery catheter. The first delivery catheter carries a first stent. The first stent comprises a proximal stent and a distal stent. The first delivery catheter also has a proximal elongate shaft with a proximal and a distal end, and a distal elongate shaft with a proximal and distal end. The proximal elongate shaft comprises a proximal expandable member with the proximal stent disposed thereover, and the distal elongate shaft comprises a distal expandable member with the distal stent disposed thereover. The proximal and distal expandable members are disposed adjacent the distal end of the first delivery catheter. The proximal and distal expandable members each have a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the collapsed configuration profile. The proximal and distal expandable members are independently expandable of one another. The second delivery catheter carries a second stent, and also has a second elongate shaft with a proximal and a distal end, and a second expandable member with the second stent disposed thereover. The second expandable member is disposed adjacent the distal end of the second elongate shaft. The second expandable member has a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the profile in the collapsed configuration. The second expandable member is independently expandable of the proximal and the distal expandable members. The third delivery catheter carries a third stent. The third delivery catheter also has a third elongate shaft with a proximal and a distal end, and a third expandable member with the third stent disposed thereover. The third expandable member is disposed adjacent the distal end of the third elongate shaft. The third expandable member has a collapsed configuration and a radially expanded configuration. The collapsed configuration has a profile suitable for advancement through a blood vessel, and the expanded configuration has a larger profile than the profile in the collapsed configuration. The third expandable member is independently expandable of the second expandable member, and the proximal and the distal expandable members.

These and other embodiments are described in further detail in the following description related to the appended drawing figures.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates an exemplary embodiment of a system for treating a bifurcation.

FIG. 2 illustrates an exemplary embodiment of a stent delivery system for treating a bifurcation.

FIG. 3A illustrates a perspective view of two notched stents that form a side hole.

FIG. 3B illustrates a flat, unrolled view of the stents in FIG. 3A.

FIG. 3C illustrates a perspective view of a side hole formed by notching one stent in a pair of adjacent stents.

FIGS. 3D-3E illustrate how various stent geometries may conform to a bifurcated vessel.

FIGS. 4A-4J illustrate an exemplary method of treating a bifurcation.

FIG. 5 illustrates another exemplary method of treating a bifurcation.

FIGS. 6A-6J illustrate an exemplary method of stenting a bifurcation.

FIG. 7 illustrates another exemplary method of stenting a bifurcation.

FIG. 8 illustrates an exemplary balloon configuration.

FIGS. 9A-9B illustrate an alternative embodiment of a balloon configuration.

FIGS. 10A-10B illustrate an exemplary embodiment of stent delivery system for treating trifurcated vessels.

DETAILED DESCRIPTION OF THE INVENTION

The present invention relates to medical devices and methods, and more particularly to stent and dilatation delivery systems for treating bifurcated vessels having a main branch and a side branch. However, this is not intended to be limiting, and one of skill in the art will appreciate that the devices and methods described herein may be used to treat other regions of the body.

The scientific community is slowly moving away from a main branch vs. side branch model and nomenclature. It is now well accepted that a “mother” vessel bifurcates into two “daughter vessels,” that are anatomically after the carina. The vessel that appears to be the continuation of the mother vessel is usually less angulated. The other vessel may be commonly referred to as the side branch, or a daughter vessel. Therefore, in this specification, the terms “main branch,” “trunk,” or “mother vessel” may be used interchangeably. Also in this specification, the terms “side branch vessel” and “daughter vessel” may also be used interchangeably. The terms “main branch stent,” “trunk stent,” or “mother stent” are interchangeable, and the term “side branch stent” is also interchangeable with the term “daughter stent.” In the case where a main branch vessel bifurcates into two equally sized branches, one of the branches may still be considered to be the main branch or mother vessel, and the other branch may be considered a side branch or daughter vessel.

Systems for Treating a Bifurcation

Referring now to FIG. 1, a system 100 for treating bifurcations comprises a first catheter 101 and a second catheter 125. The first catheter includes a first elongate shaft 102 having a proximal region 104 and a distal region 112. A proximal expandable member, here a balloon 108, and a distal expandable member, also a balloon 110 are disposed near the distal region of the first catheter 101. A gap 113 separates the proximal expandable member 108 from the distal expandable member 110. The proximal expandable member is disposed on the first elongate shaft 102, and the distal expandable member 110 is disposed over an extended portion 112 of the first shaft 102. The extended portion 112 may be a stepped down, reduced diameter portion of the first shaft 102, or it may be a separate shaft that is coupled with the first shaft 102. The extended portion may also be a coextruded shaft that extends parallel to the first shaft. The extended portion 112 may be fixed relative to the first shaft 102, or it may also be slidably movable relative to the first shaft 102. Proximal 114a and distal 114b radiopaque markers may be disposed adjacent the distal expandable member 110 in order to allow a physician to visualize balloon location during fluoroscopy. Simi-

larly, proximal **129a** and distal **129b** radiopaque markers may be disposed adjacent the proximal balloon **108**. The markers are preferably positioned at the proximal and distal working ends of the respective balloon. An inflation lumen (not illustrated) allows the balloon **110** to be inflated from the proximal end of the first catheter. A guidewire lumen **118** extends from a distal port **115** at the distal end of the extension shaft to the proximal portion of the catheter and terminates in a Y-connector **120** having two ports **122**, **124** with fittings such as Luer fittings. The Luer fittings may be used to fluidly couple the catheter with a balloon inflation device such as an Inflator, a syringe, medical tubing, or other devices commonly used during a catheterization procedure. The guidewire lumen **118** is coupled with port **122**, and thus the first catheter may be delivered over a guidewire GW which slidably passes from the distal port **115**, through the extended portion **112**, though the first catheter **102**, and exits proximal port **122**. This configuration is commonly referred to as an over-the-wire configuration. While not illustrated, one of skill in the art will also appreciate that the proximal guidewire port may also be located anywhere along the first delivery catheter, and in some preferred embodiments the proximal port **122** is located closer to the distal port **115** than the proximal end of the first catheter. This configuration is commonly referred to as Rx, or rapid exchange configuration. Both balloons may be inflated independently of one another, and thus balloon **108** has its own inflation lumen (not illustrated) which is passes through the first elongate shaft **102** and terminates at hub **116** which has a fitting such a Luer fitting to allow an inflation device such as an Inflator to be fluidly coupled to the catheter. Both the proximal and distal expandable members may be expanded from a collapsed configuration having a low profile suitable for intravascular delivery to a target treatment site such as a bifurcated vessel, to a radially expanded configuration in which the balloons engage the walls of the target treatment site, such as a blood vessel wall.

The second catheter **125** also has an elongate shaft **126** having a proximal portion and a distal portion. An expandable member **134**, here a balloon, is disposed on the elongate shaft **126**, near it's distal end. A proximal **136a** and distal **136b** radiopaque marker may be coupled to the shaft **126** and aligned with the balloon **134** so that a physician may visualize the balloon under fluoroscopy. The radiopaque markers **136a**, **136b** are preferably located at the proximal and the distal working ends of the balloon **134**. A proximal connector **130** is coupled to the proximal end of the shaft **126** and allows a syringe, inflation device, medical tubing, or other device to be fluidly coupled with an inflation lumen (not shown) which extends along the elongate shaft **126** and is fluidly coupled to the expandable member **134**. A guidewire lumen **128** extends from a distal port **135** to a proximal port **132**. In preferred embodiments, the proximal port **132** is closer to the distal port **135** than the proximal end of the elongate shaft **126**. This configuration is often referred to as Rx or rapid exchange. The guidewire lumen may also optionally extend out the proximal end of the shaft to provide a catheter having what is commonly referred to as an over-the-wire configuration. In preferred embodiments, shaft **126** may extend slidably through a lumen **106** in the shaft **102** of the first catheter **101** so that the balloon **134** may be advanced or retracted relative to the distal balloon **110**. In other embodiments, shaft **126** may be fixedly attached to shaft **102** with no relative movement between the two catheters. Balloon **134** may be expanded from a collapsed configuration having a low profile suitable for intravascular delivery to a target treatment site such as a bifurcated vessel, to a radially expanded configuration in which the balloons engage the walls of the target treatment site, such as a blood

vessel wall. Any of the balloons **108**, **110**, **134** may be compliant, non-compliant, or semi-compliant. Moreover, any of the balloons **108**, **110**, **134** may have a substantially constant diameter, or they may be tapered to match the contours of a vessel. In preferred embodiments, the balloons are tapered and non-compliant.

FIG. 2 illustrates another catheter system **200** for treating a bifurcation. In this exemplary embodiment, catheter system **200** is similar to the system **100** of FIG. 1, with the major difference being that system **100** also includes three stents **152**, **154**, **158**.

The first catheter carries a first stent which is comprised of two discrete stents, a proximal stent **152** is disposed over the proximal balloon **108** on the first catheter **101**, and a distal stent **154** is disposed over the distal balloon **110**. A proximal end of the distal stent **154** abuts with a distal end of the proximal stent **108**. The abutting ends of the two stents are formed so that when the two stents abut one another, a side hole **156** is created, allowing the second elongate shaft **126** to pass therethrough. Exemplary embodiments of the stent side hole are disclosed in greater detail below. The side hole **156** is preferably disposed about midway between the proximal and distal stents **152**, **154**, however, by changing stent lengths or by further modifying the abutting ends of the stents, the side hole may be disposed anywhere between the ends of the two stents **152**, **154**. A second stent **158**, comprised of a single stent is disposed over balloon **134** on the second delivery catheter. Other aspects of delivery system **200** generally take the same form as those previously described above with respect to catheter system **100**. The stents **152**, **154**, **158** are preferably balloon expandable, but may also be self-expanding, or combinations of balloon expandable and self-expanding. The stents **152**, **154**, **158** are radially expandable from a collapsed or crimped configuration having a profile adapted for intravascular delivery through a vessel, to an expanded configuration in which the stents engage and provide support for a target tissue such as a vessel wall. The stents may have any length, and in preferred embodiments, the proximal stent **152**, and the distal stent **154** are substantially the same length. One of skill in the art will appreciate that this is not intended to be limiting, and stent length is dependent upon the length of the target tissue being treated.

FIG. 3A illustrates a perspective view of the two stents **152**, **154** in FIG. 2, with the delivery catheter removed for clarity. A proximal portion of distal stent **154** includes a notched region **154a**, and similarly a distal portion of the proximal stent **152** also includes a notched portion **152a**. The notched regions may be sized so that when the proximal portion of stent **154** abuts with the distal portion of stent **152**, the two notched regions form a side hole **156** through which the second catheter **126** may pass. FIG. 3B illustrates the stents **152**, **154** in the unrolled, flattened configuration to more clearly illustrate how the notched region may be cut into the stent. In this exemplary embodiment, the notched region is half of an ellipse, but in other embodiments, the notched region may be circular, rectangular, or other shapes may be employed. Also, in still other embodiments, the notch may be cut out of only one of the two abutting stents. FIG. 3C illustrates an exemplary embodiment of two stents **152**, **154** that form a side hole **156** when the two stents abut one another. In this embodiment, a single notch **154a** is cut out of only one of the stents, here stent **154** in this embodiment, although the notch could also be cut out of stent **152**.

For conventional cylindrical stents **175** having orthogonal ends, placement in a side branch may result in a region **178** of the side branch that is remains unscaffolded, as seen in FIG. 3D. Providing a stent **180** having a beveled end **182** may allow

11

the stent to more accurately conform to the side branch anatomy, thereby providing more uniform scaffolding as seen in FIG. 3E.

Methods of Treating a Bifurcation

FIGS. 4A-4J illustrate an exemplary method of treating a bifurcated vessel using the system 100 of FIG. 1. FIG. 4A illustrates the basic anatomy of stenotic lesion at a bifurcated vessel. The blood vessel BV includes a main branch MB and a side branch SB. At the bifurcation B, the vessel bifurcates into the side branch SB and a downstream portion of the main branch MB. The carina C is a keel-shaped ridge, process, or anatomical part of the bifurcation. A stenotic lesion L such as plaque, calcified deposits, or other narrowing material is disposed in the side branch, as well as in the main branch upstream and downstream of the bifurcation. The ostium O is the opening from the main branch MB into the side branch SB.

In FIG. 4B a guidecatheter or introducer catheter IC is introduced into the patient's vasculature, preferably percutaneously, or via cutdown. The introducer catheter IC is then advanced toward the target treatment area at the bifurcation. Two guidewires GW are then advanced through the introducer catheter. One guidewire is further advanced into the side branch SB past the side branch lesion L, and the other guidewire is advanced further into the main branch downstream of the main branch lesion L.

FIG. 4C shows the bifurcation treatment system 100 of FIG. 1 being advanced through the introducer catheter IC, over both guidewires GW. Both catheters 101, 125 are advanced distally until they engage the carina C, resisting further distal advancement. Both catheters may be advanced slightly distally, or retracted slightly proximally such that the first catheter 101 is positioned in the main branch MB with the proximal balloon 108 at least partially upstream of the bifurcation B, and the distal balloon 110 is at least partially downstream of the bifurcation B. Both balloons 108, 110 of course will be aligned with the lesion L in the main branch MB. The second catheter 125 is positioned in the side branch SB, preferably such that balloon 134 is slightly distal to the side branch lesion L.

FIG. 4D illustrates an optional step wherein the second catheter 125 is proximally retracted through a lumen (not shown) in the first catheter 101 so that proximal radiopaque marker 136a on the second catheter 125 is aligned with proximal radiopaque marker 129a on the first catheter 101. This may be seen in the partial cutaway in FIG. 4D. Thus, a portion of shaft 126 slides under proximal balloon 108 and through the shaft 102 of the first catheter 101. Furthermore, this ensures alignment of balloon 134 with the side branch lesion L, with the ostium of the side branch, and with the proximal 108 and distal 110 balloons. This aspect of the procedure, as well as any other aspect of the procedure may be visualized using fluoroscopy, ultrasound, or other imaging techniques suitable for catheterization procedures.

Once the balloons on both catheters are properly aligned with the lesion, the bifurcation, and with one another, the balloons may be radially expanded in any order in order to treat the lesion L. FIG. 4E illustrates a preferred first inflation wherein the balloon 134 on the second catheter 125 is expanded against the lesion L in the side branch SB. The balloon 134 may be inflated with saline, contrast media, combinations thereof, or with other fluids. The balloons are inflated to a pressure high enough to compact the plaque into the vessel wall, preferably greater than 10 atmospheres, more preferably 10 to 20 atmospheres, and even more preferably 15 to 25 atmospheres. Of course, one of skill in the art will appreciate that this pressure is not limiting, and a physician

12

may inflate the balloon to any desired pressure. After the balloon is inflated once, or twice, or more, it is deflated, and the plaque will be substantially reduced since it is pressed into the vessel wall, thereby reducing the stenotic lesion L.

FIG. 4F illustrates another preferred step, wherein the proximal balloon 108 is expanded next, after expansion of the balloon 134 in the side branch SB. The proximal balloon may be inflated with similar fluids and pressures as previously described above. This reduces the plaque in the main branch near the bifurcation, and upstream of the bifurcation. FIG. 4G illustrates the next preferred step wherein the distal balloon 110 is expanded using similar fluids and pressures as described above. Expansion of both proximal 108 and distal 110 balloons is a modified "kissing" balloon technique. Even though the balloons 108, 110 are separated by a gap, after inflation, the proximal end of the distal balloon 110 expands toward and abuts the distal end of the proximal balloon 108 which also advances toward the other balloon. Additional details on this are disclosed below in FIGS. 8 and 9A-9B. Expanding both the proximal and distal balloons 108, 110 ensures that the lesion L in the main branch, both upstream and downstream of the bifurcation is uniformly dilated. Optionally, the side branch balloon 134 may also be simultaneously expanded (not illustrated) so that all three balloons "kiss" one another.

After the lesion has been successfully dilated, both proximal and distal balloons 108, 110 (and side branch balloon 134, if also expanded) are deflated as illustrated in FIG. 4H. In FIG. 4I, both catheters 101, 125 are proximally retracted away from the bifurcation, and removed from the patient's body. Finally, in FIG. 4J, both guidewires GW and the introducer guidecatheter IC are also proximally retracted away from the bifurcation and removed from the patient's body. The blockage in the lumen is now substantially reduced, thereby improving blood flow across the bifurcation.

The exemplary method described above is not intended to be limiting. One of skill in the art will appreciate that a number of variations or changes may also be made. For example, any one or more of the balloons may be coated with a therapeutic agent such as an anti-restenosis drug like rapamycin, everolimus, biolimus A9, other analogs of rapamycin, or paclitaxel to help reduce restenosis. Moreover, any order or combination of balloon inflation may also be used. For example, the proximal and distal balloons may be expanded prior to expansion of the side branch balloon, or the distal balloon may be inflated before the proximal balloon. Other variations may include simultaneous inflation of the side branch balloon with the proximal balloon, or simultaneous inflation of the side branch balloon and the distal balloon. Any number of permutations are contemplated.

Additionally, in an alternative embodiment shown in FIG. 5, the distal balloon 110 of the first catheter 101 may be advanced into the side branch SB while the proximal balloon 108 remains in the main branch MB. The balloon 134 on the second catheter 125 may then be advanced into the main MB branch at least partially downstream of the bifurcation. Inflation of the balloons may follow any of the number of permutations discussed above.

FIGS. 6A-6J illustrate an exemplary method of stenting a bifurcation using the delivery system 200 previously described in FIG. 2 above. FIG. 6A illustrates the basic anatomy of stenotic lesion at a bifurcated vessel. The blood vessel BV includes a main branch MB and a side branch SB. At the bifurcation B, the vessel bifurcates into the side branch SB and a downstream portion of the main branch MB. The carina C is a keel-shaped ridge, process, or anatomical part of the bifurcation. A stenotic lesion L such as plaque, calcified

deposits, or other narrowing material is disposed in the side branch, as well as in the main branch upstream and downstream of the bifurcation. The ostium O is the opening from the main branch MB into the side branch SB.

In FIG. 6B a guidecatheter or introducer catheter IC is introduced into the patient's vasculature, preferably percutaneously, or via cutdown. The introducer catheter IC is then advanced toward the target treatment area at the bifurcation. Two guidewires GW are then advanced through the introducer catheter. One guidewire is further advanced into the side branch SB past the side branch lesion L, and the other guidewire is advanced further into the main branch downstream of the main branch lesion L.

FIG. 6C shows the bifurcation treatment system 200 of FIG. 2 being advanced through the introducer catheter IC, over both guidewires GW. Both catheters 101, 125 are advanced distally until they engage the carina C, resisting further distal advancement. Both catheters may be advanced slightly distally, or retracted slightly proximally such that the first catheter 101 is positioned in the main branch MB with the proximal stent 152 at least partially upstream of the bifurcation B, and the distal stent 154 is at least partially downstream of the bifurcation B. Both stents 152, 154 of course will be aligned with the lesion L in the main branch MB. Furthermore, the notched regions 152a, 154a forming the side hole 156 will also be aligned with the ostium to the side branch. The second catheter 125 is positioned in the side branch SB, preferably such that stent 158 is slightly distal to the side branch lesion L. In this embodiment, the stents 152, 154, 158 are preferably balloon expandable. However, they may also be self-expanding, or combinations of balloon expandable and self-expanding.

FIG. 6D illustrates an optional step wherein the second catheter 125 is proximally retracted through a lumen (not shown) in the first catheter 101 so that proximal radiopaque marker 136a on the second catheter 125 is aligned with proximal radiopaque marker 129a on the first catheter 101. This may be seen in the partial cutaway in FIG. 6D. Thus, a portion of shaft 126 slides under proximal balloon 108, under proximal stent 152, and through the shaft 102 of the first catheter 101. Furthermore, this ensures alignment of stent 158 with the side branch lesion L, with the ostium of the side branch, and with the proximal 152 and distal 154 balloons. This aspect of the procedure, as well as any other aspect of the procedure may be visualized using fluoroscopy, ultrasound, or other imaging techniques suitable for catheterization procedures.

Once the stents on both catheters are properly aligned with the lesion, the bifurcation, and with one another, the balloons may be radially expanded thereby expanding the stents to treat the lesion. FIG. 6E illustrates a preferred first inflation wherein the balloon 134 on the second catheter 125 is expanded, thereby expanding stent 158 into the lesion L in the side branch SB. The balloon 134 may be inflated with saline, contrast media, combinations thereof, or with other fluids. The balloons are inflated to similar pressures as those previously described above. Of course, one of skill in the art will appreciate that these pressures are not limiting, and a physician may inflate the balloon to any desired pressure. After the stent is expanded into the lesion, the balloon 134 is deflated. A second post-dilation may also be performed if necessary to further tack the stent into position.

FIG. 6F illustrates another preferred step, wherein the proximal balloon 108 is expanded next so as to radially expand the proximal stent 152 into the lesion L around the lesion and slightly upstream of the bifurcation. Expansion of stent 152 is performed after expansion of stent 158 in the side

branch SB. The proximal balloon may be inflated with similar fluids and pressures as previously described above. FIG. 6G illustrates the next preferred step wherein the distal balloon 110 is expanded using similar fluids and pressures as described above, thereby expanding distal stent 154. The distal balloon is inflated while the proximal balloon is inflated. Expansion of both proximal 108 and distal 110 balloons is a modified "kissing" balloon technique. Even though the balloons 108, 110 are separated by a gap, after inflation, the proximal end of the distal balloon 110 expands toward and abuts the distal end of the proximal balloon 108 which also advances toward the other balloon. Additional details on this are disclosed below in reference to FIGS. 8, and 9A-9B. This helps ensure that the distal end of the proximal stent 152 abuts the proximal end of the distal stent 154, and that the side hole 156 abuts the proximal end of the side branch stent 158, thereby ensuring that the stent fully covers and scaffolds the bifurcation. Additionally, expanding both the proximal and distal balloons 108, 110 ensures that the proximal and distal stents 152, 154 are expanded uniformly in the main branch, both upstream and downstream of the bifurcation. Optionally, the side branch balloon 134 may also be simultaneously expanded (not illustrated) so that all three balloons "kiss" with one another.

After the lesion has been successfully stented, both proximal and distal balloons 108, 110 (and side branch balloon 134, if also expanded) are deflated as illustrated in FIG. 6H. In FIG. 6I, both catheters 101, 125 are proximally retracted away from the bifurcation, and removed from the patient's body. Finally, in FIG. 6J, both guidewires GW and the introducer guidecatheter IC are also proximally retracted away from the bifurcation and removed from the patient's body. The blockage in the lumen is now substantially reduced and scaffolded, thereby improving blood flow across the bifurcation.

The exemplary method described above is not intended to be limiting. One of skill in the art will appreciate that a number of variations or changes may also be made. For example, any one or more of the balloons, stents, or combinations of balloons/stents may be coated with a therapeutic agent such as an anti-restenosis drug like rapamycin, everolimus, biolimus A9, other analogs of rapamycin, or paclitaxel to help reduce restenosis. Moreover, any order or combination of balloon/stent expansion may be employed. For example, the proximal and distal balloons/stents may be expanded prior to expansion of the side branch balloon/stent, or the distal balloon/stent may be inflated before the proximal balloon/stent. Other variations may include simultaneous expansion of the side branch balloon/stent with the proximal balloon/stent, or simultaneous inflation of the side branch balloon/stent and the distal balloon/stent. Any number of permutations are contemplated.

Additionally, in an alternative embodiment shown in FIG. 7, the distal stent 154 of the first catheter 101 may be advanced into the side branch SB while the proximal stent 152 remains in the main branch MB. The stent 158 on the second catheter 125 may then be advanced into the main MB branch at least partially downstream of the bifurcation. Inflation of the balloons may follow any of the number of permutations discussed above.

Exemplary Balloon Configurations

FIG. 8 illustrates one exemplary balloon configuration that may be used in any of the systems or method described above. Catheter shaft 302 includes a proximal balloon 304 and a distal balloon 306 coupled to the shaft 302. Both proximal and distal balloons 304, 306 have standard proximal tapers 308 and distal tapers 310. The tapered regions 308, 310 allow

15

the balloon to be fixedly coupled to shaft **302** with a fluid tight seal. This may be accomplished by ultrasonic welding, adhesively bonding, suture wrapping, or other techniques known to those in the art. While this configuration is promising, the gap **308** separating the proximal and distal balloons **304**, **306** will remain even after both balloons are inflated. Thus, a section of the vessel may remain undilated, or unstented, which is not optimal.

FIG. **9A** illustrates another exemplary balloon configuration that may overcome some of the shortcomings of the previous embodiment. Shaft **302** includes a proximal balloon **304a** and a distal balloon **306a**. The proximal end **312a** and the distal end **314a** of each balloon is everted and attached to the shaft using similar techniques as those described above. In the unexpanded configuration of FIG. **9A**, a gap **308** still exists when the balloons are uninflated. However, when both balloons **304a**, **306a** are inflated, because of the everted ends, the proximal end of each balloon will tend to move proximally, and the distal end of each balloon will also tend to move distally, as indicated by the arrows. Thus, the distal end of the proximal balloon **304a** will move toward and abut the proximal end of the distal balloon **306a**. This reduces or eliminates the gap **308** between the two balloons. Therefore, the vessel will be more uniformly dilated or stented. Also, in the case where stents are mounted over the balloons, the ends of the stents will also tend to move toward one another, therefore the gap between adjacent stents will also tend to close resulting in more uniform stenting.

Exemplary Stent Delivery Systems for Treating Trifurcations

The embodiments described above are preferably used to treat bifurcated vessels. However, the basic embodiment may be expanded upon in order to treat trifurcated vessels such that those with a main branch and two side branches. FIGS. **10A-10B** illustrate one exemplary embodiment of a stent delivery system that may be used to stent a trifurcated vessel. Stent delivery system **1002** includes a first side branch stent delivery catheter **1004** and a second side branch stent delivery catheter **1006**. Also, the main branch stent delivery catheter includes a proximal balloon **1012** with a stent **1010** disposed thereover, and a distal balloon with a stent **1018** disposed thereover and coupled to a central shaft **1008**. The central shaft includes at least three lumens sized to accommodate the shafts of the first and second side branch catheters, and the main branch shaft. The shafts may be slidably disposed in the lumens, or they may be fixed. The first side branch stent delivery catheter includes a balloon **1030** and stent **1031** disposed thereover near the catheter distal end. It is disposed in a rapid exchange lumen of the main shaft such that the proximal port **1026** is closer to the distal end of the catheter than the proximal end of the catheter. The second side branch catheter is similarly configured and includes a balloon **1032** and a stent **1033** disposed thereover adjacent the distal end of the catheter. The second side branch catheter is disposed in a rapid exchange lumen of the main shaft such that the proximal port is closer to the distal end of the catheter than the proximal end. The main branch catheter includes proximal balloon **1012** having a proximal taper **1016** and a distal everted end **1014** that allows the distal end of the balloon to expand distally toward the distal main branch balloon upon inflation. In alternative embodiments, both ends of balloon **1012** may be tapered, everted, or the proximal end may be everted and the distal end may be tapered. The distal main branch balloon preferably includes a distal taper **1020** and a proximal everted end **1022** that moves proximally toward the proximal main branch balloon upon inflation. A gap **1034** separates the proximal main branch stent from the distal main branch stent,

16

thereby creating a space for the first and second side branch catheters to extend therepast. The gap may be created with the notches or other stent geometries previously described above, with the exception that two notches are required to form two gaps. During delivery, the two side branch catheters may be slidably disposed in the lumens of the main branch catheter. Upon reaching the target trifurcated vessel, the two side branch catheters may be distally extended from the lumens and exposed, passing through the gap **1034** between the proximal and distal main branch stents. The balloons may be independently inflatable thereby allowing inflation in any order to deploy stents upstream and downstream of the trifurcation, and in the two sidebranches. Kissing balloons may also be used. In an alternative embodiments, one or more of the balloons may not include a stent, and thus the a portion of the trifurcation may be dilated and a portion of the trifurcation may be stented.

While the above is a complete description of the preferred embodiments of the invention, various alternatives, modifications, and equivalents may be used. Therefore, the above description should not be taken as limiting the scope of the invention which is defined by the appended claims.

What is claimed is:

1. A method for treating a bifurcated vessel in a patient, the bifurcated vessel having a main branch and a side branch, said method comprising:

providing a first delivery catheter comprising a proximal first expandable member, a distal second expandable member, a proximal first stent, and a distal second stent, wherein the proximal first expandable member and distal second expandable member are disposed close to or at a distal end of the first delivery catheter,

wherein the proximal first stent and the distal second stent are discrete stents, the proximal first stent disposed over the proximal first expandable member, and the distal second stent disposed over the distal second expandable member, and

wherein a distal portion of the proximal first stent comprises a notched region, and a proximal portion of the distal second stent comprises a notched region, the notched regions being cut out portions of the distal portion of the proximal first stent and the proximal portion of the distal second stent, respectively, and the notched regions being adjacent one another to form a side hole in the proximal first stent and the distal second stent;

providing a second delivery catheter comprising a third expandable member and a third stent, the third expandable member disposed close to or at a distal end of the second delivery catheter,

wherein the third stent is disposed over the third expandable member, and

wherein the second delivery catheter passes through the side hole in the proximal first stent and the distal second stent;

advancing the first delivery catheter and the second delivery catheter toward the bifurcation;

positioning the proximal first stent, the distal second stent, and the third stent at the bifurcation such that the proximal first stent is disposed in the main branch, the distal second stent is disposed in the side branch, and the third stent is disposed in the main branch downstream of the bifurcation,

wherein the side hole in the proximal first stent and the distal second stent is aligned with the main branch and faces downstream of the bifurcation;

17

radially expanding the distal second stent from a collapsed configuration to an expanded configuration;
 radially expanding the proximal first stent from a collapsed configuration to an expanded configuration; and
 radially expanding the third stent from a collapsed configuration to an expanded configuration.

2. The method of claim 1, wherein positioning the proximal first stent, the distal second stent, and the third stent comprises advancing the first delivery catheter and the second delivery catheter until one or more of the delivery catheters engage a carina of the bifurcation.

3. The method of claim 1, wherein radially expanding the distal second stent comprises expanding the distal second stent to engage a wall of the side branch.

4. The method of claim 1, wherein radially expanding the distal second stent comprises expanding the distal second expandable member.

5. The method of claim 4, wherein the distal second expandable member comprises a balloon, and expanding the distal second expandable member comprises inflating the balloon.

6. The method of claim 1, wherein radially expanding the proximal first stent comprises expanding the proximal first stent to engage a wall of the main branch.

7. The method of claim 1, wherein radially expanding the proximal first stent comprise expanding the proximal first expandable member.

8. The method of claim 7, wherein the proximal first expandable member comprises a balloon, and expanding the proximal first expandable member comprises inflating the balloon.

9. The method of claim 1, wherein the proximal first stent is radially expanded before radial expansion of the distal second stent.

18

10. The method of claim 1, wherein radially expanding the third stent comprises expanding the third stent to engage a wall of the main branch.

11. The method of claim 10, wherein radially expanding the third stent comprises expanding the third expandable member.

12. The method of claim 11, wherein the third expandable member comprises a balloon, and expanding the third expandable member comprises inflating the balloon.

13. The method of claim 1, wherein the third stent is radially expanded after radial expansion of the proximal first stent and the distal second stent.

14. The method of claim 1, further comprising proximally retracting the second delivery catheter so that a proximal end of the third stent is aligned with the side hole in the proximal first stent and the distal second stent.

15. The method of claim 14, wherein proximally retracting the second delivery catheter comprises aligning a radiopaque marker on the second delivery catheter with a radiopaque marker on the first delivery catheter.

16. The method of claim 14, wherein proximally retracting the second delivery catheter comprises sliding the second delivery catheter under a portion of the proximal first stent.

17. The method of claim 16, wherein proximally retracting the second delivery catheter comprises sliding the second delivery catheter through the side hole in the proximal first stent and the distal second stent.

18. The method of claim 1, wherein a proximal portion of the third stent abuts a portion of the proximal first stent and a portion of the distal second stent, after radial expansion of the proximal first stent, the distal second stent, and the third stent.

19. The method of claim 18, wherein the distal portion of the proximal first stent abuts the proximal portion of the distal second stent after radial expansion thereof.

* * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 9,254,210 B2
APPLICATION NO. : 13/796466
DATED : February 9, 2016
INVENTOR(S) : Henry Bourang

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

In item (71), in “Applicant”, in Column 1, Line 1, delete “Systems,” and insert --Systems-- therefor

In item (73), in “Assignee”, in Column 1, Line 1, delete “Systems,” and insert --Systems-- therefor

Signed and Sealed this
Twenty-first Day of April, 2020

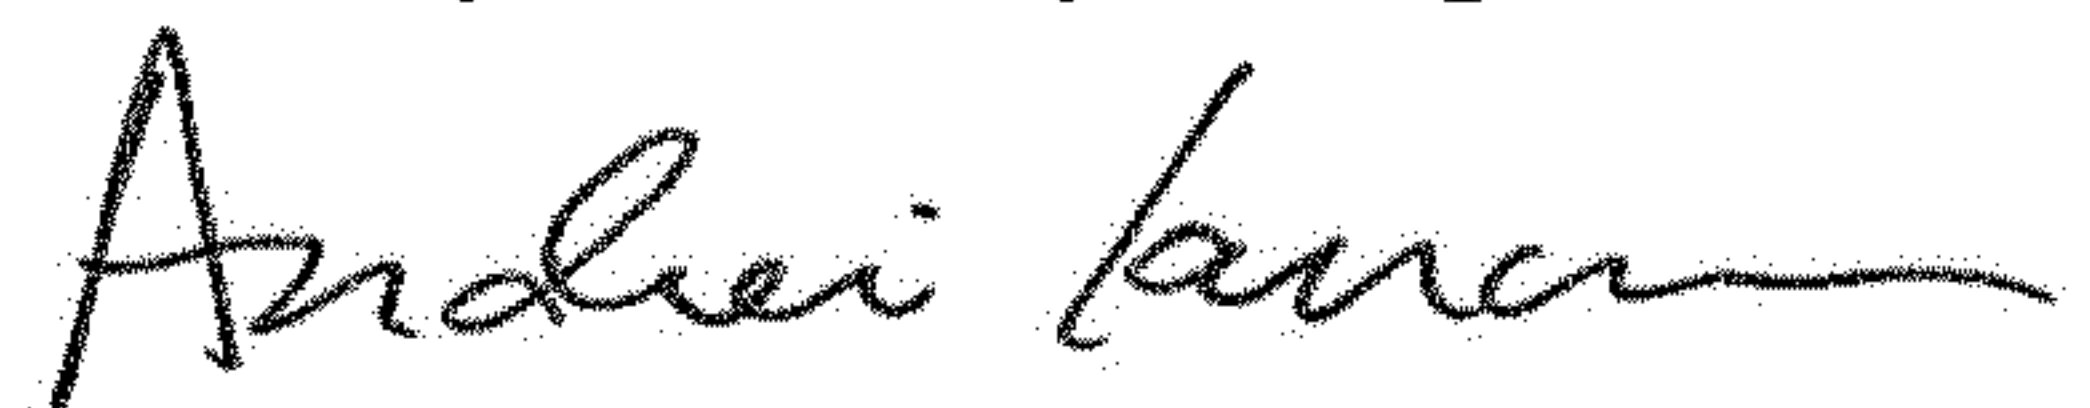

Andrei Iancu
Director of the United States Patent and Trademark Office