



US009352151B2

(12) **United States Patent**
Wijting et al.

(10) **Patent No.:** **US 9,352,151 B2**
(45) **Date of Patent:** ***May 31, 2016**

(54) **METHOD AND APPARATUS FOR APPLYING
NEUROMUSCULAR ELECTRICAL
STIMULATION**

(71) Applicant: **Encore Medical Asset Corporation,**
Henderson, NV (US)

(72) Inventors: **Yorick Wijting**, Hixson, TN (US);
Jeffrey K. Pohl, Soddy Daisy, TN (US)

(73) Assignee: **Encore Medical Asset Corporation,**
Vista, CA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 138 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **14/144,256**

(22) Filed: **Dec. 30, 2013**

(65) **Prior Publication Data**

US 2014/0188013 A1 Jul. 3, 2014

Related U.S. Application Data

(63) Continuation of application No. 11/706,455, filed on
Feb. 13, 2007, now Pat. No. 8,620,438.

(51) **Int. Cl.**
A61N 1/00 (2006.01)
A61N 1/36 (2006.01)
A61N 7/00 (2006.01)

(52) **U.S. Cl.**
CPC **A61N 1/36003** (2013.01); **A61N 7/00**
(2013.01)

(58) **Field of Classification Search**
CPC A61N 1/04; A61N 1/0404; A61N 1/0452;
A61N 1/00; A61N 1/0456; A61N 1/36003;
A61N 1/36139

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,263,205 A 11/1941 Conrad
3,344,792 A 10/1967 Offner et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE 3216911 11/1983
DE 19545238 5/1997

(Continued)

OTHER PUBLICATIONS

Ilic, Milan et al. "A Programmable Electronic Stimulator for FES
Systems" IEEE Transactions on Rehabilitation Engineering, vol. 2,
No. 4, Dec. 1994.

(Continued)


Primary Examiner — Mallika D Fairchild

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson &
Bear LLP

(57) **ABSTRACT**

A method and apparatus for applying neuromuscular electri-
cal stimulation to an agonist/antagonist muscle pair to move
a limb about a joint includes generating a first pattern of
neuromuscular electrical stimulation pulses for output
through a first channel to a first pair of electrodes and gener-
ating a second pattern of neuromuscular stimulation pulses
for output through a second channel to a second pair of
electrodes. The first pair of electrodes are attached to the
agonist muscle of the agonist/antagonist muscle pair, and the
second pair of electrodes are attached to the antagonist
muscle. A first pattern of electrical stimulation pulses is trans-
mitted through the first pair of electrodes to the agonist
muscle at a first intensity level to initiate contraction of the
agonist muscle, and then at a second intensity level which is
less than the first intensity level to continue contraction of the
agonist muscle. A second pattern of electrical stimulation
pulses is transmitted through the second pair of electrodes to
the antagonist muscle at a first intensity level to reduce the
acceleration of the limb, and then at a second intensity level
which is less than the first intensity level to regulate the
movement of the limb.

21 Claims, 10 Drawing Sheets

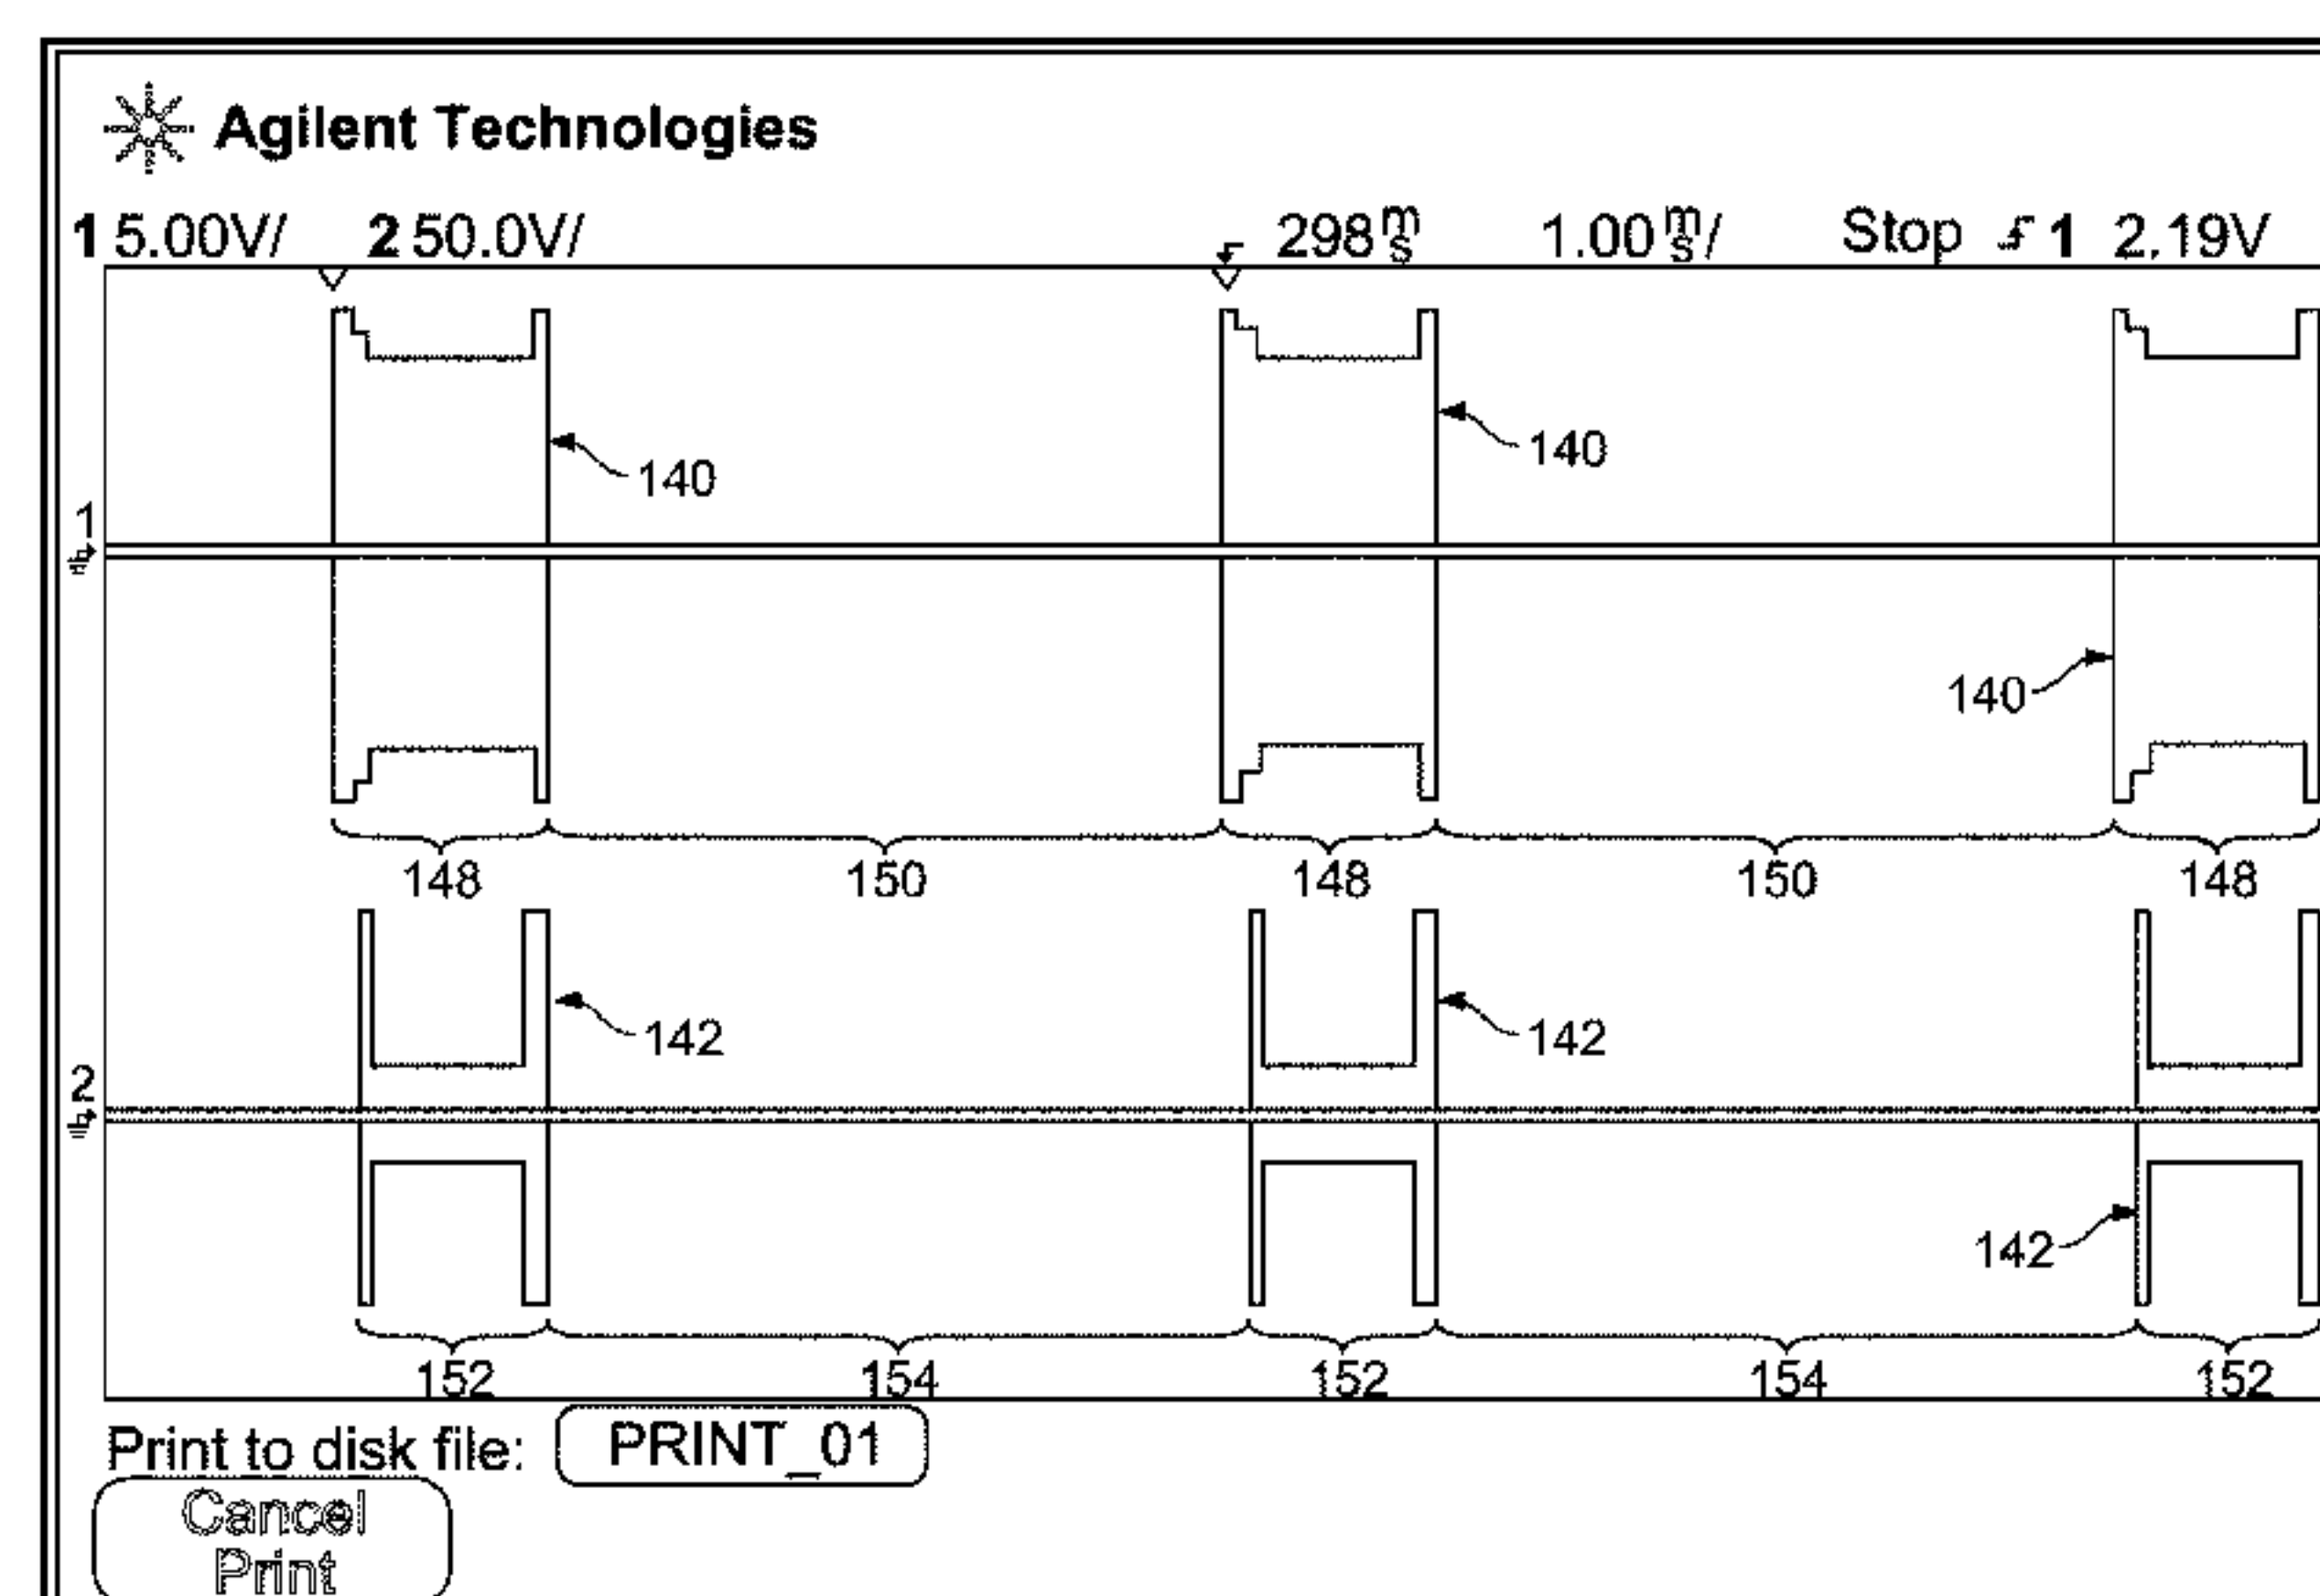

(56)

References Cited

U.S. PATENT DOCUMENTS

3,628,538 A 12/1971 Vincent et al.
 3,810,457 A 5/1974 Bottcher et al.
 3,895,639 A 7/1975 Rodler
 3,918,459 A 11/1975 Horn
 4,019,518 A 4/1977 Maurer et al.
 4,068,669 A 1/1978 Niemi
 4,088,141 A 5/1978 Niemi
 4,164,740 A 8/1979 Constant
 4,165,750 A 8/1979 Aleev et al.
 4,177,819 A 12/1979 Kofsky et al.
 4,256,116 A 3/1981 Meretsky et al.
 4,324,253 A 4/1982 Greene et al.
 4,342,317 A 8/1982 Axelgaard
 4,363,324 A 12/1982 Kusserow
 4,372,319 A 2/1983 Ichinomiya et al.
 4,390,023 A 6/1983 Rise
 4,392,496 A 7/1983 Stanton
 4,408,609 A 10/1983 Axelgaard
 4,503,863 A 3/1985 Katims
 4,535,777 A 8/1985 Castel
 4,569,352 A 2/1986 Petrofsky et al.
 4,580,339 A 4/1986 Ioffe
 4,582,063 A 4/1986 Mickiewicz et al.
 4,586,495 A 5/1986 Petrofsky
 4,614,178 A 9/1986 Harlt et al.
 4,632,117 A 12/1986 James
 4,640,286 A 2/1987 Thomson
 4,664,118 A 5/1987 Batters
 4,669,477 A 6/1987 Ober
 4,690,145 A 9/1987 King-Smith et al.
 4,706,674 A 11/1987 Dieken et al.
 4,769,881 A 9/1988 Pedigo et al.
 4,785,813 A 11/1988 Petrofsky
 4,803,988 A 2/1989 Thomson
 4,805,636 A 2/1989 Barry et al.
 4,811,742 A 3/1989 Hassel et al.
 4,848,347 A 7/1989 Hall
 4,887,603 A 12/1989 Morawetz et al.
 4,919,139 A 4/1990 Brodard
 4,926,865 A 5/1990 Oman
 4,976,264 A 12/1990 Petrofsky
 4,977,895 A 12/1990 Tannenbaum
 4,996,987 A 3/1991 Petrofsky
 5,041,974 A 8/1991 Walker et al.
 5,048,522 A 9/1991 Petrofsky
 5,067,478 A 11/1991 Berlant
 5,067,495 A 11/1991 Brehm
 5,070,873 A 12/1991 Graupe et al.
 5,081,989 A 1/1992 Graupe et al.
 5,092,329 A 3/1992 Graupe et al.
 5,113,176 A 5/1992 Harris
 5,117,826 A 6/1992 Bartelt et al.
 5,123,413 A 6/1992 Hasegawa et al.
 5,131,401 A 7/1992 Westenskow et al.
 5,161,530 A 11/1992 Gamble
 5,178,156 A 1/1993 Takishima et al.
 5,184,617 A 2/1993 Harris et al.
 5,233,987 A 8/1993 Fabian et al.
 5,285,781 A 2/1994 Brodard
 5,300,096 A 4/1994 Hall et al.
 5,350,414 A 9/1994 Kolen
 5,397,338 A 3/1995 Grey et al.
 5,413,550 A 5/1995 Castel
 5,507,788 A 4/1996 Lieber
 5,512,057 A 4/1996 Reiss et al.
 5,514,165 A 5/1996 Malaugh et al.
 5,540,235 A 7/1996 Wilson
 5,540,735 A 7/1996 Wingrove
 5,562,718 A 10/1996 Palermo
 5,653,739 A 8/1997 Maurer et al.
 5,732,401 A 3/1998 Conway
 5,748,845 A 5/1998 Labun et al.
 5,755,745 A 5/1998 McGraw et al.
 5,775,331 A 7/1998 Raymond et al.
 5,776,171 A 7/1998 Peckham et al.

5,776,173 A 7/1998 Madsen, Jr. et al.
 5,782,893 A 7/1998 Dennis, III
 5,800,458 A 9/1998 Wingrove
 5,817,138 A 10/1998 Suzuki
 5,836,995 A 11/1998 MGraw et al.
 RE35,987 E 12/1998 Harris et al.
 5,873,900 A 2/1999 Maurer et al.
 5,954,758 A 9/1999 Peckham et al.
 5,961,542 A 10/1999 Agarwala
 5,967,975 A 10/1999 Ridgeway
 5,980,435 A 11/1999 Joutras et al.
 6,026,328 A 2/2000 Peckham et al.
 6,029,090 A 2/2000 Herbst
 6,041,259 A 3/2000 Agarwala et al.
 6,044,303 A 3/2000 Agarwala et al.
 RE36,690 E 5/2000 McGraw et al.
 6,064,911 A 5/2000 Wingrove
 6,086,525 A 7/2000 Davey et al.
 6,113,552 A 9/2000 Shimazu et al.
 6,146,335 A 11/2000 Gozani
 6,233,472 B1 5/2001 Bennett et al.
 6,285,906 B1 9/2001 Ben-Haim et al.
 6,292,692 B1 9/2001 Skelton et al.
 6,324,432 B1 11/2001 Rigaux et al.
 6,393,328 B1 5/2002 McGraw et al.
 6,432,074 B1 8/2002 Ager et al.
 6,445,955 B1 9/2002 Michelson et al.
 6,560,487 B1 5/2003 McGraw et al.
 6,564,103 B2 5/2003 Fischer et al.
 6,584,358 B2 6/2003 Carter et al.
 6,609,031 B1 8/2003 Law et al.
 6,612,984 B1 9/2003 Kerr, II
 6,628,492 B2 9/2003 Akiyama et al.
 6,647,290 B2 11/2003 Wuthrich
 6,662,051 B1 12/2003 Eraker et al.
 6,675,048 B2 1/2004 McGraw et al.
 6,684,106 B2 1/2004 Herbst
 6,701,189 B2 3/2004 Fang et al.
 6,727,814 B2 4/2004 Saltzstein et al.
 6,826,429 B2 11/2004 Johnson et al.
 6,839,594 B2 1/2005 Cohen et al.
 6,845,271 B2 1/2005 Fang et al.
 6,876,883 B2 4/2005 Hurtado
 6,907,295 B2 6/2005 Gross et al.
 6,963,773 B2 11/2005 Waltman et al.
 6,988,005 B2 1/2006 McGraw et al.
 2001/0051787 A1 12/2001 Haller et al.
 2002/0165590 A1 11/2002 Crowe et al.
 2003/0036683 A1 2/2003 Kehr et al.
 2003/0065370 A1 4/2003 Lebel et al.
 2003/0074037 A1 4/2003 Moore et al.
 2003/0120323 A1 6/2003 Meadows et al.
 2004/0010291 A1 1/2004 Wagner et al.
 2004/0147975 A1 7/2004 Popovic et al.
 2004/0167585 A1 8/2004 Kovak et al.
 2005/0055054 A1 3/2005 Yu

FOREIGN PATENT DOCUMENTS

DE 4092175 7/1997
 EP 0 269 844 6/1988
 EP 0 367 338 5/1990
 EP 0 706 806 4/1996
 EP 1 095 670 5/2001
 FR 2425865 12/1979
 FR 2504807 11/1982
 JP 2004-0081676 3/2004
 WO WO 82/00414 2/1982
 WO WO 86/02567 5/1986
 WO WO 95/10323 4/1995
 WO WO 99/19019 4/1999
 WO WO 99/41682 8/1999
 WO WO 00/01055 1/2000
 WO WO 00/36900 6/2000
 WO WO 01/03768 1/2001
 WO WO 01/51122 7/2001
 WO WO 02/085452 10/2002
 WO WO 03/008038 1/2003
 WO WO 2004/011087 2/2004

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 2004/012807	2/2004
WO	WO 2004/018038	3/2004
WO	WO 2004/064915	8/2004

OTHER PUBLICATIONS

Strojnink, P., Peckham, P.H., Chapter 78 Implantable Stimulators for neuromuscular control, The Biomedical engineering handbook, Second Edition, vol. 1, Editor: Joseph D. Bronzino, CRC Press , IEEE Press.

Strojnink, P., Peckham, P.H., Chapter 78 Implantable Stimulators for neuromuscular control, pp. 78-1 to 78-3, the Biomedical engineering

handbook, Second Edition, vol. 1, Editor: Joseph D. Bronzino, CRC Press ,1999, Print ISBN: 978-0/8493-8594-0, eBook ISBN: 978-1-4200-4951-0, DOI: 10.1201/9781420049510.ch78.

“Cyclotec Pain Control Products,” Cyclotec AMT, 3 pages. Retrieved from <http://www.cyclotecamt.com/pages2/products.htm> on May 25, 2004.

“Muscle Stimulator and TENS: Very different modalities,” RS Medical, 1 page Retrieved from <http://www.rsmedical.com/products/diff/body.htm> on Apr. 27, 2004.

“Netwave,” Blue Sky Labs; 6 pages; Copyright 2003.

“RS-4i Sequential Stimulator,” 6 pages; Retrieved from <http://www.rsmedical.com/products/rs2/body.htm> on Apr. 27, 2004.

“501(k) Summary for netwave Interferential Stimulator,” Ryan Telemedicine, LLC; Jun. 12, 2003.

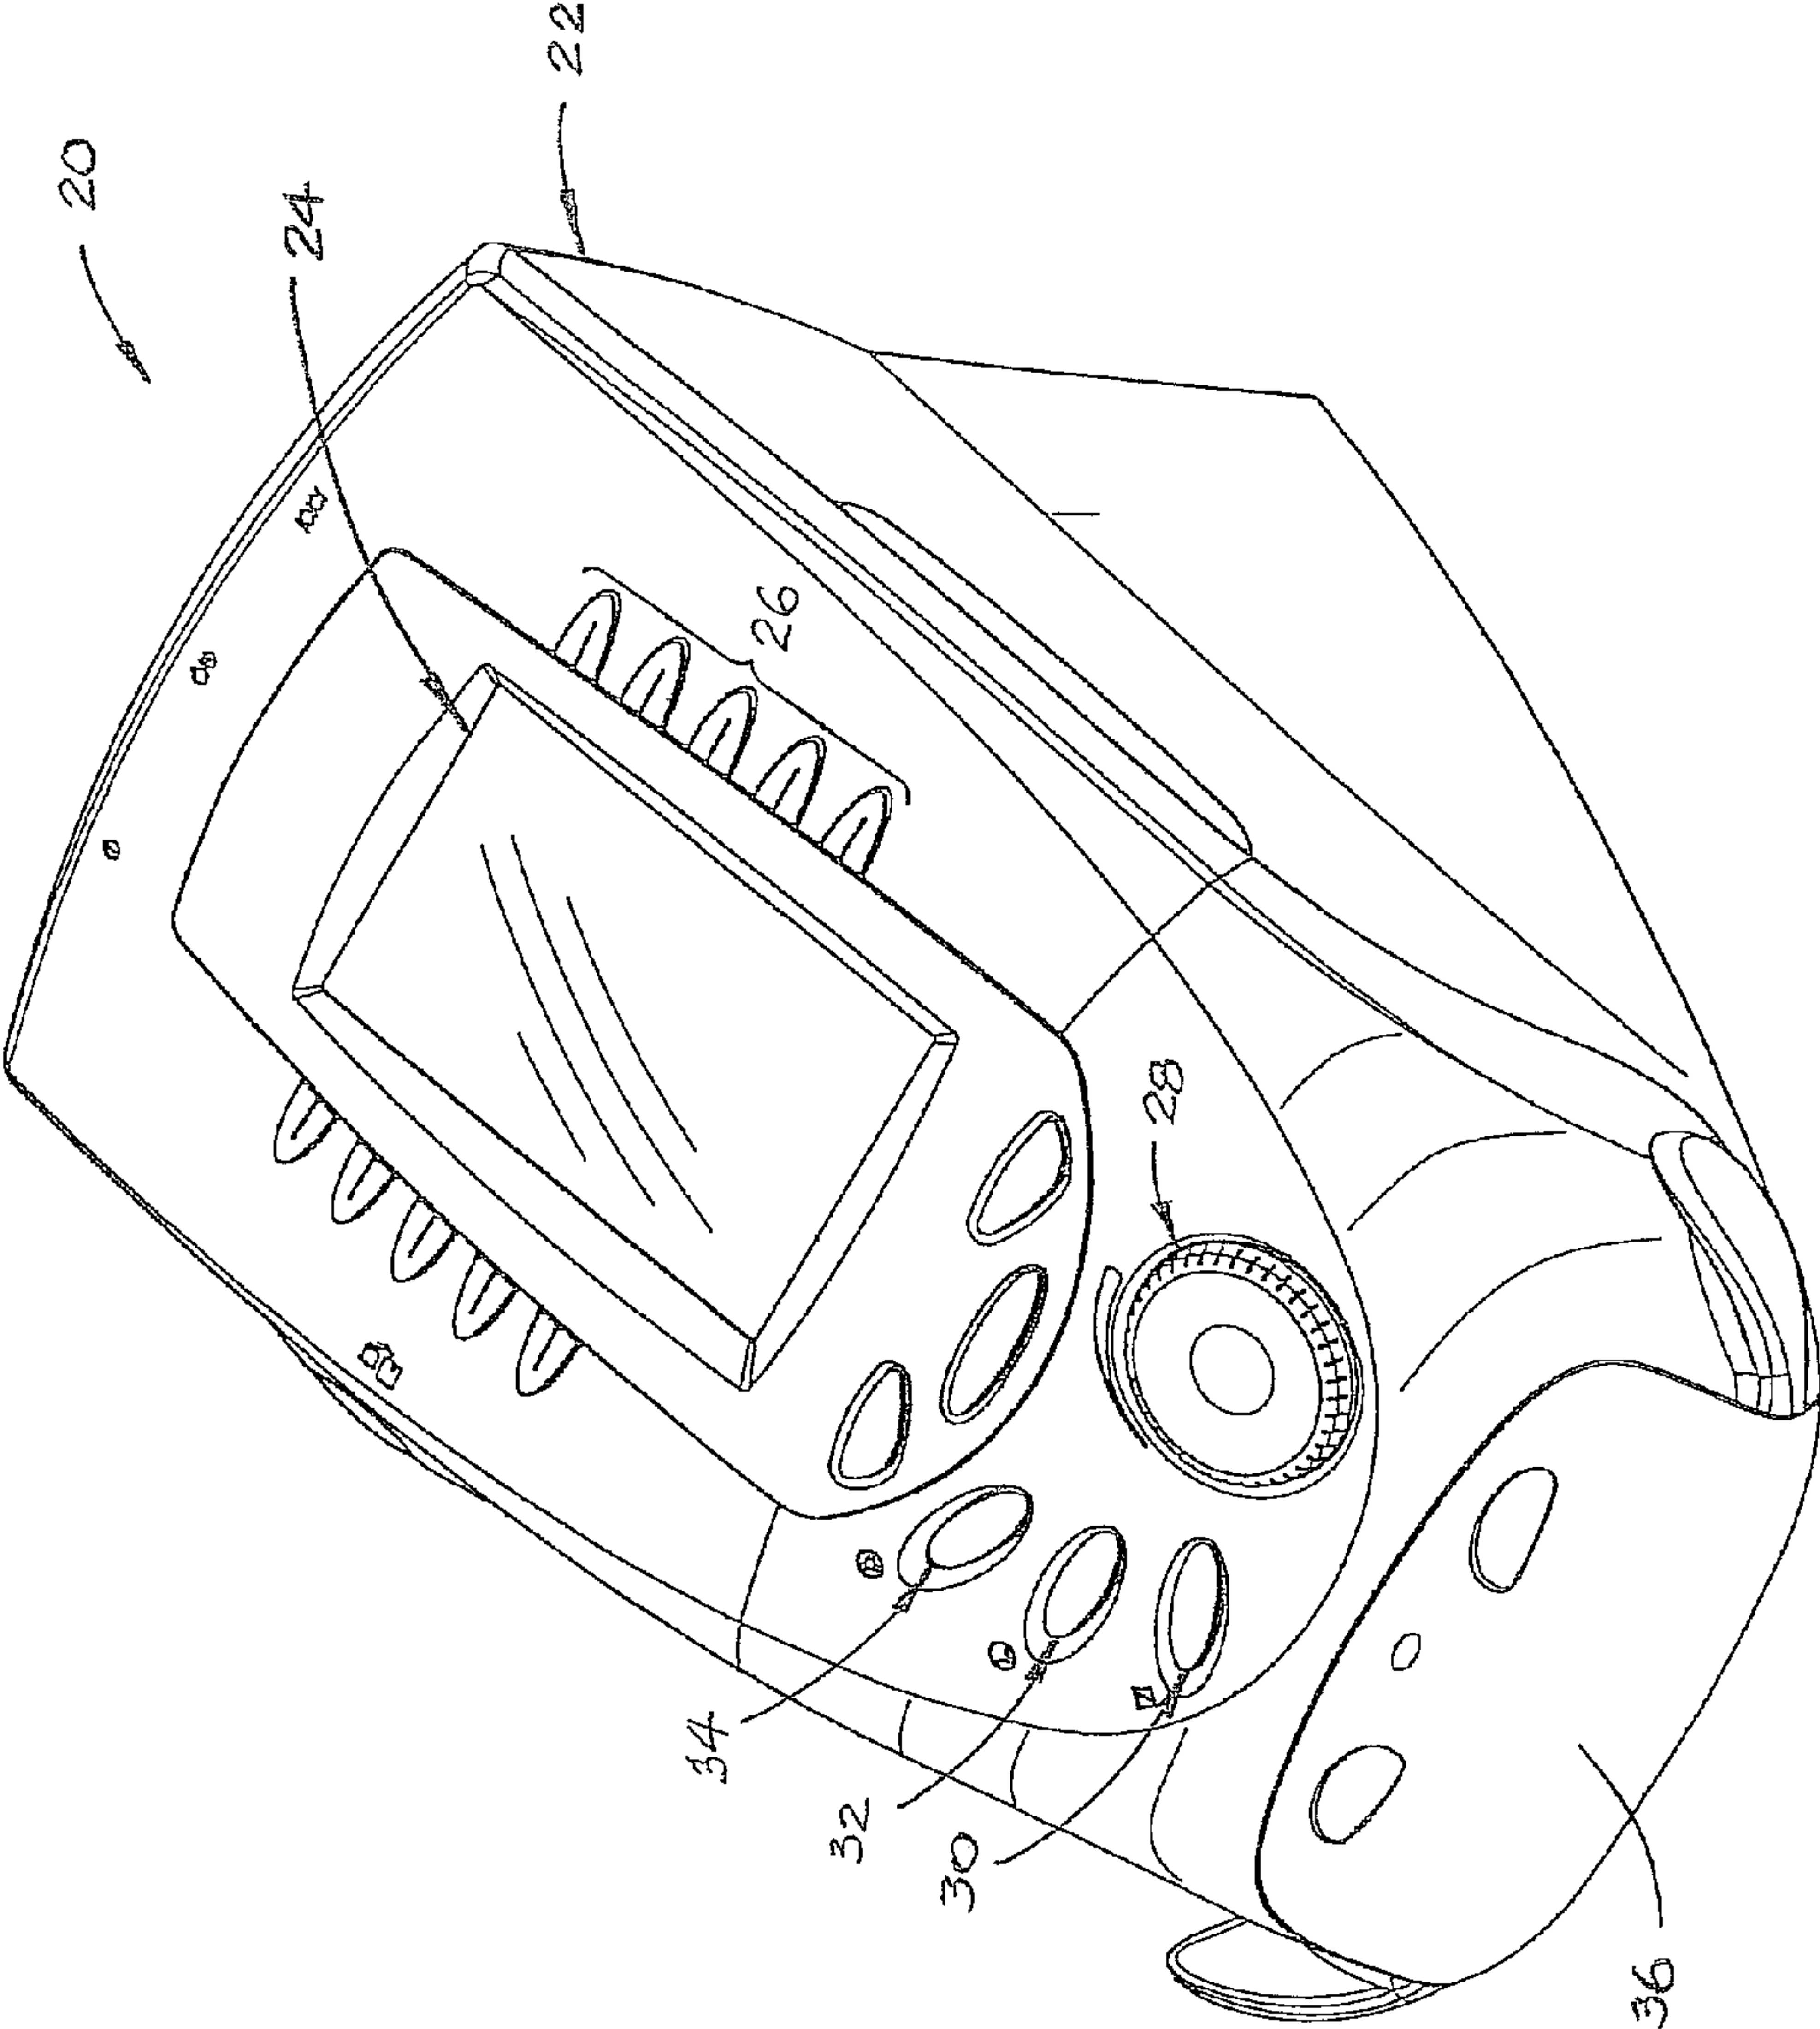


FIGURE 1

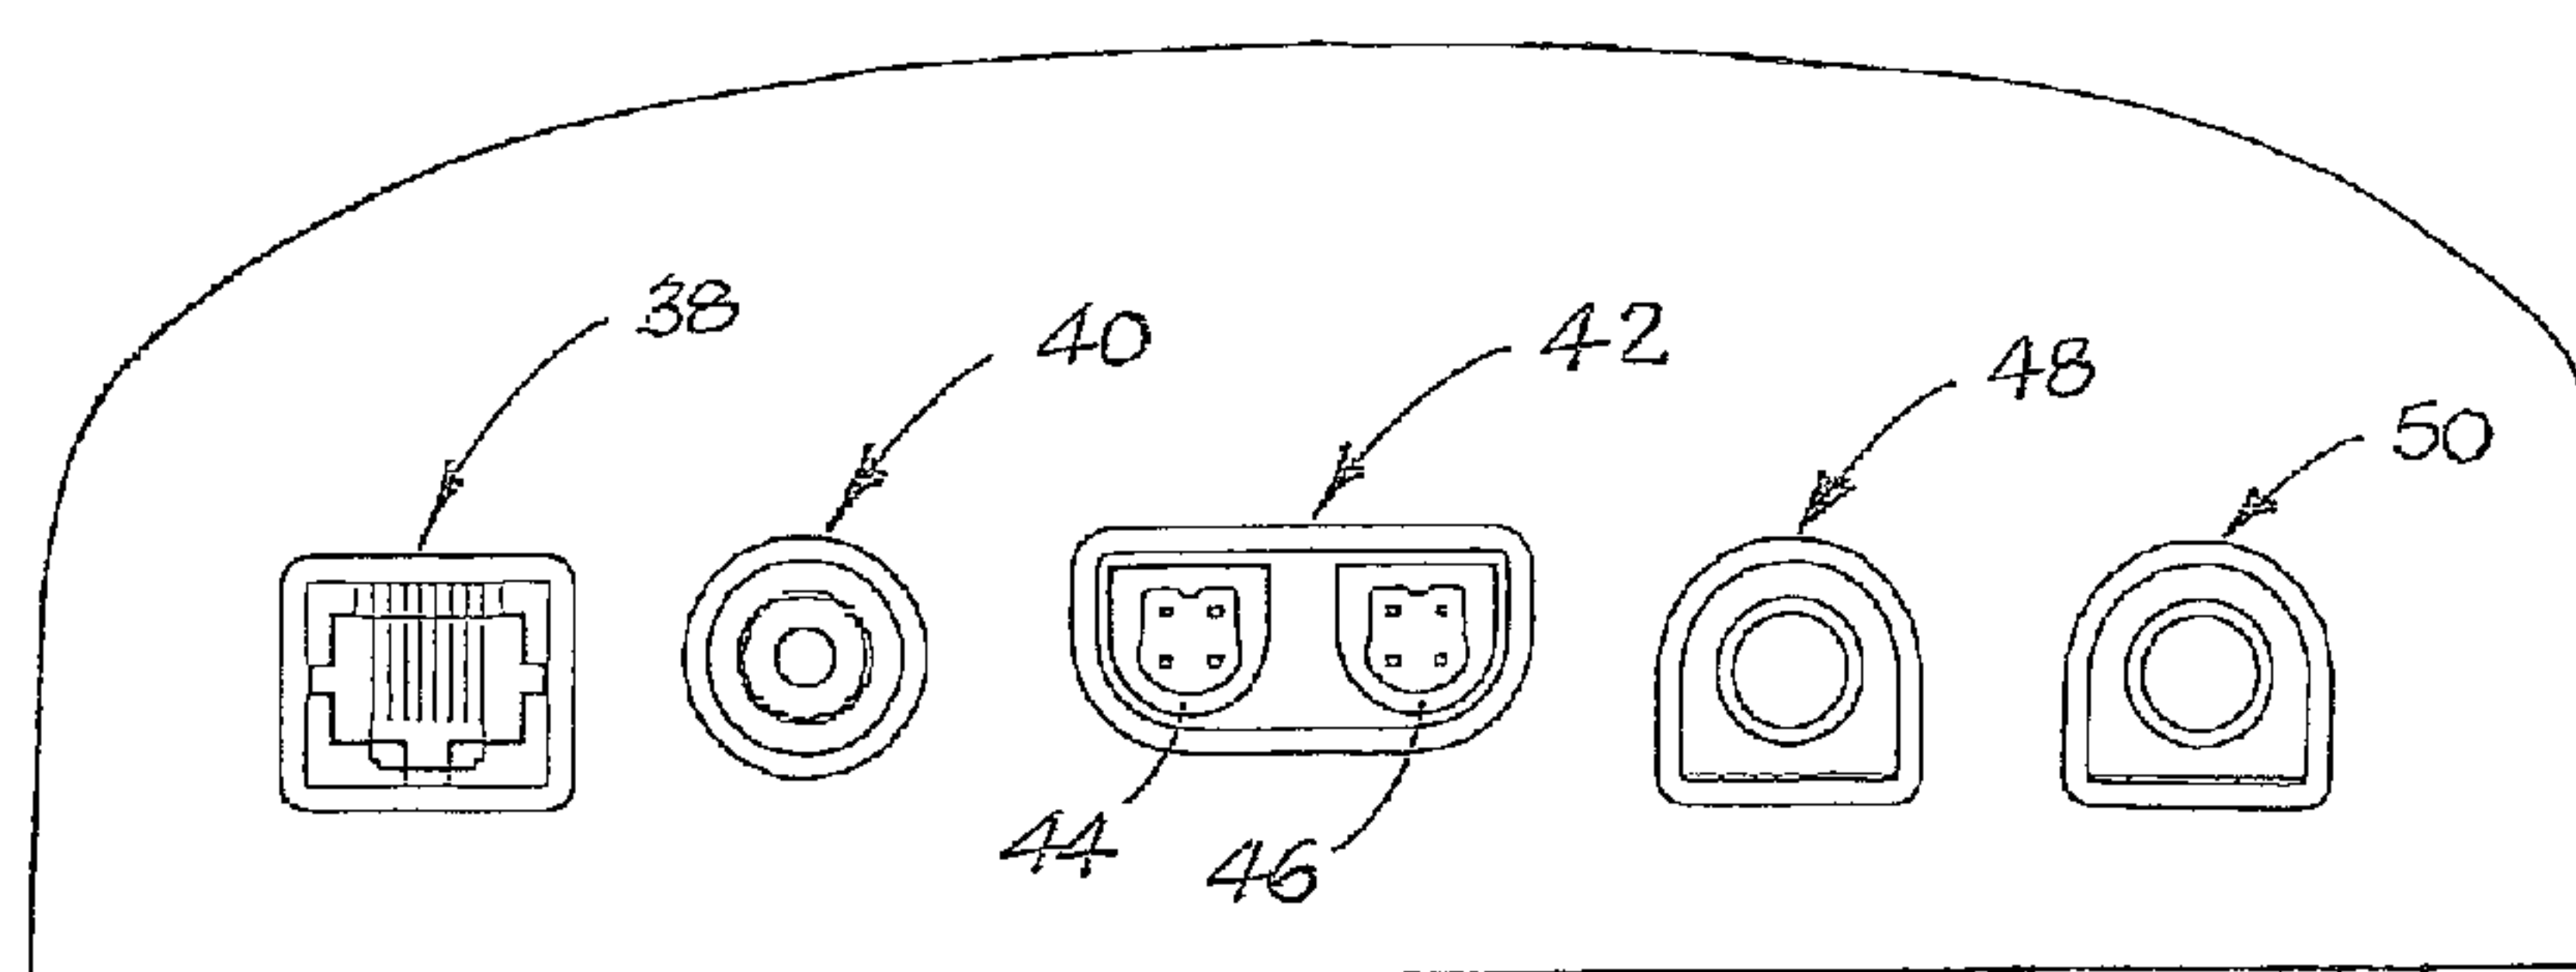


FIGURE 2

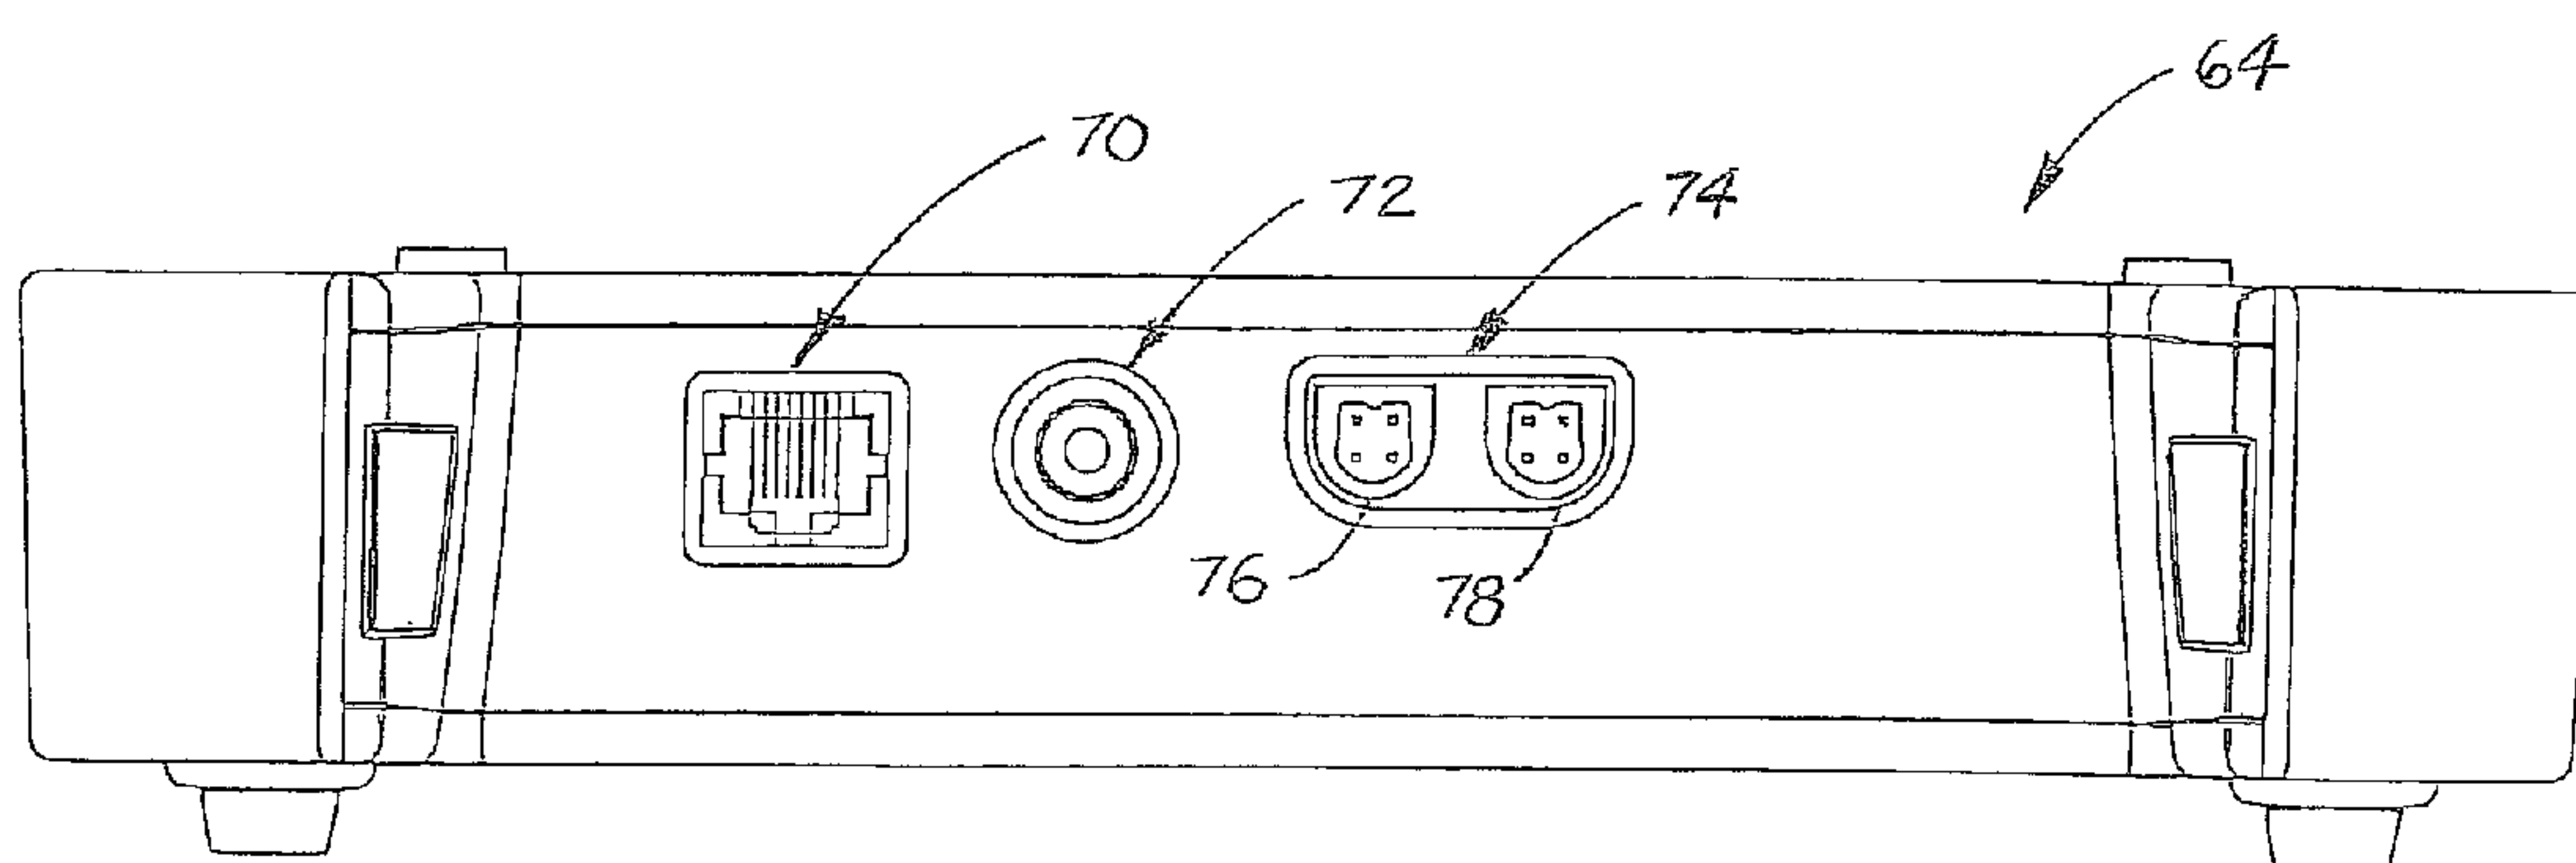


FIGURE 6

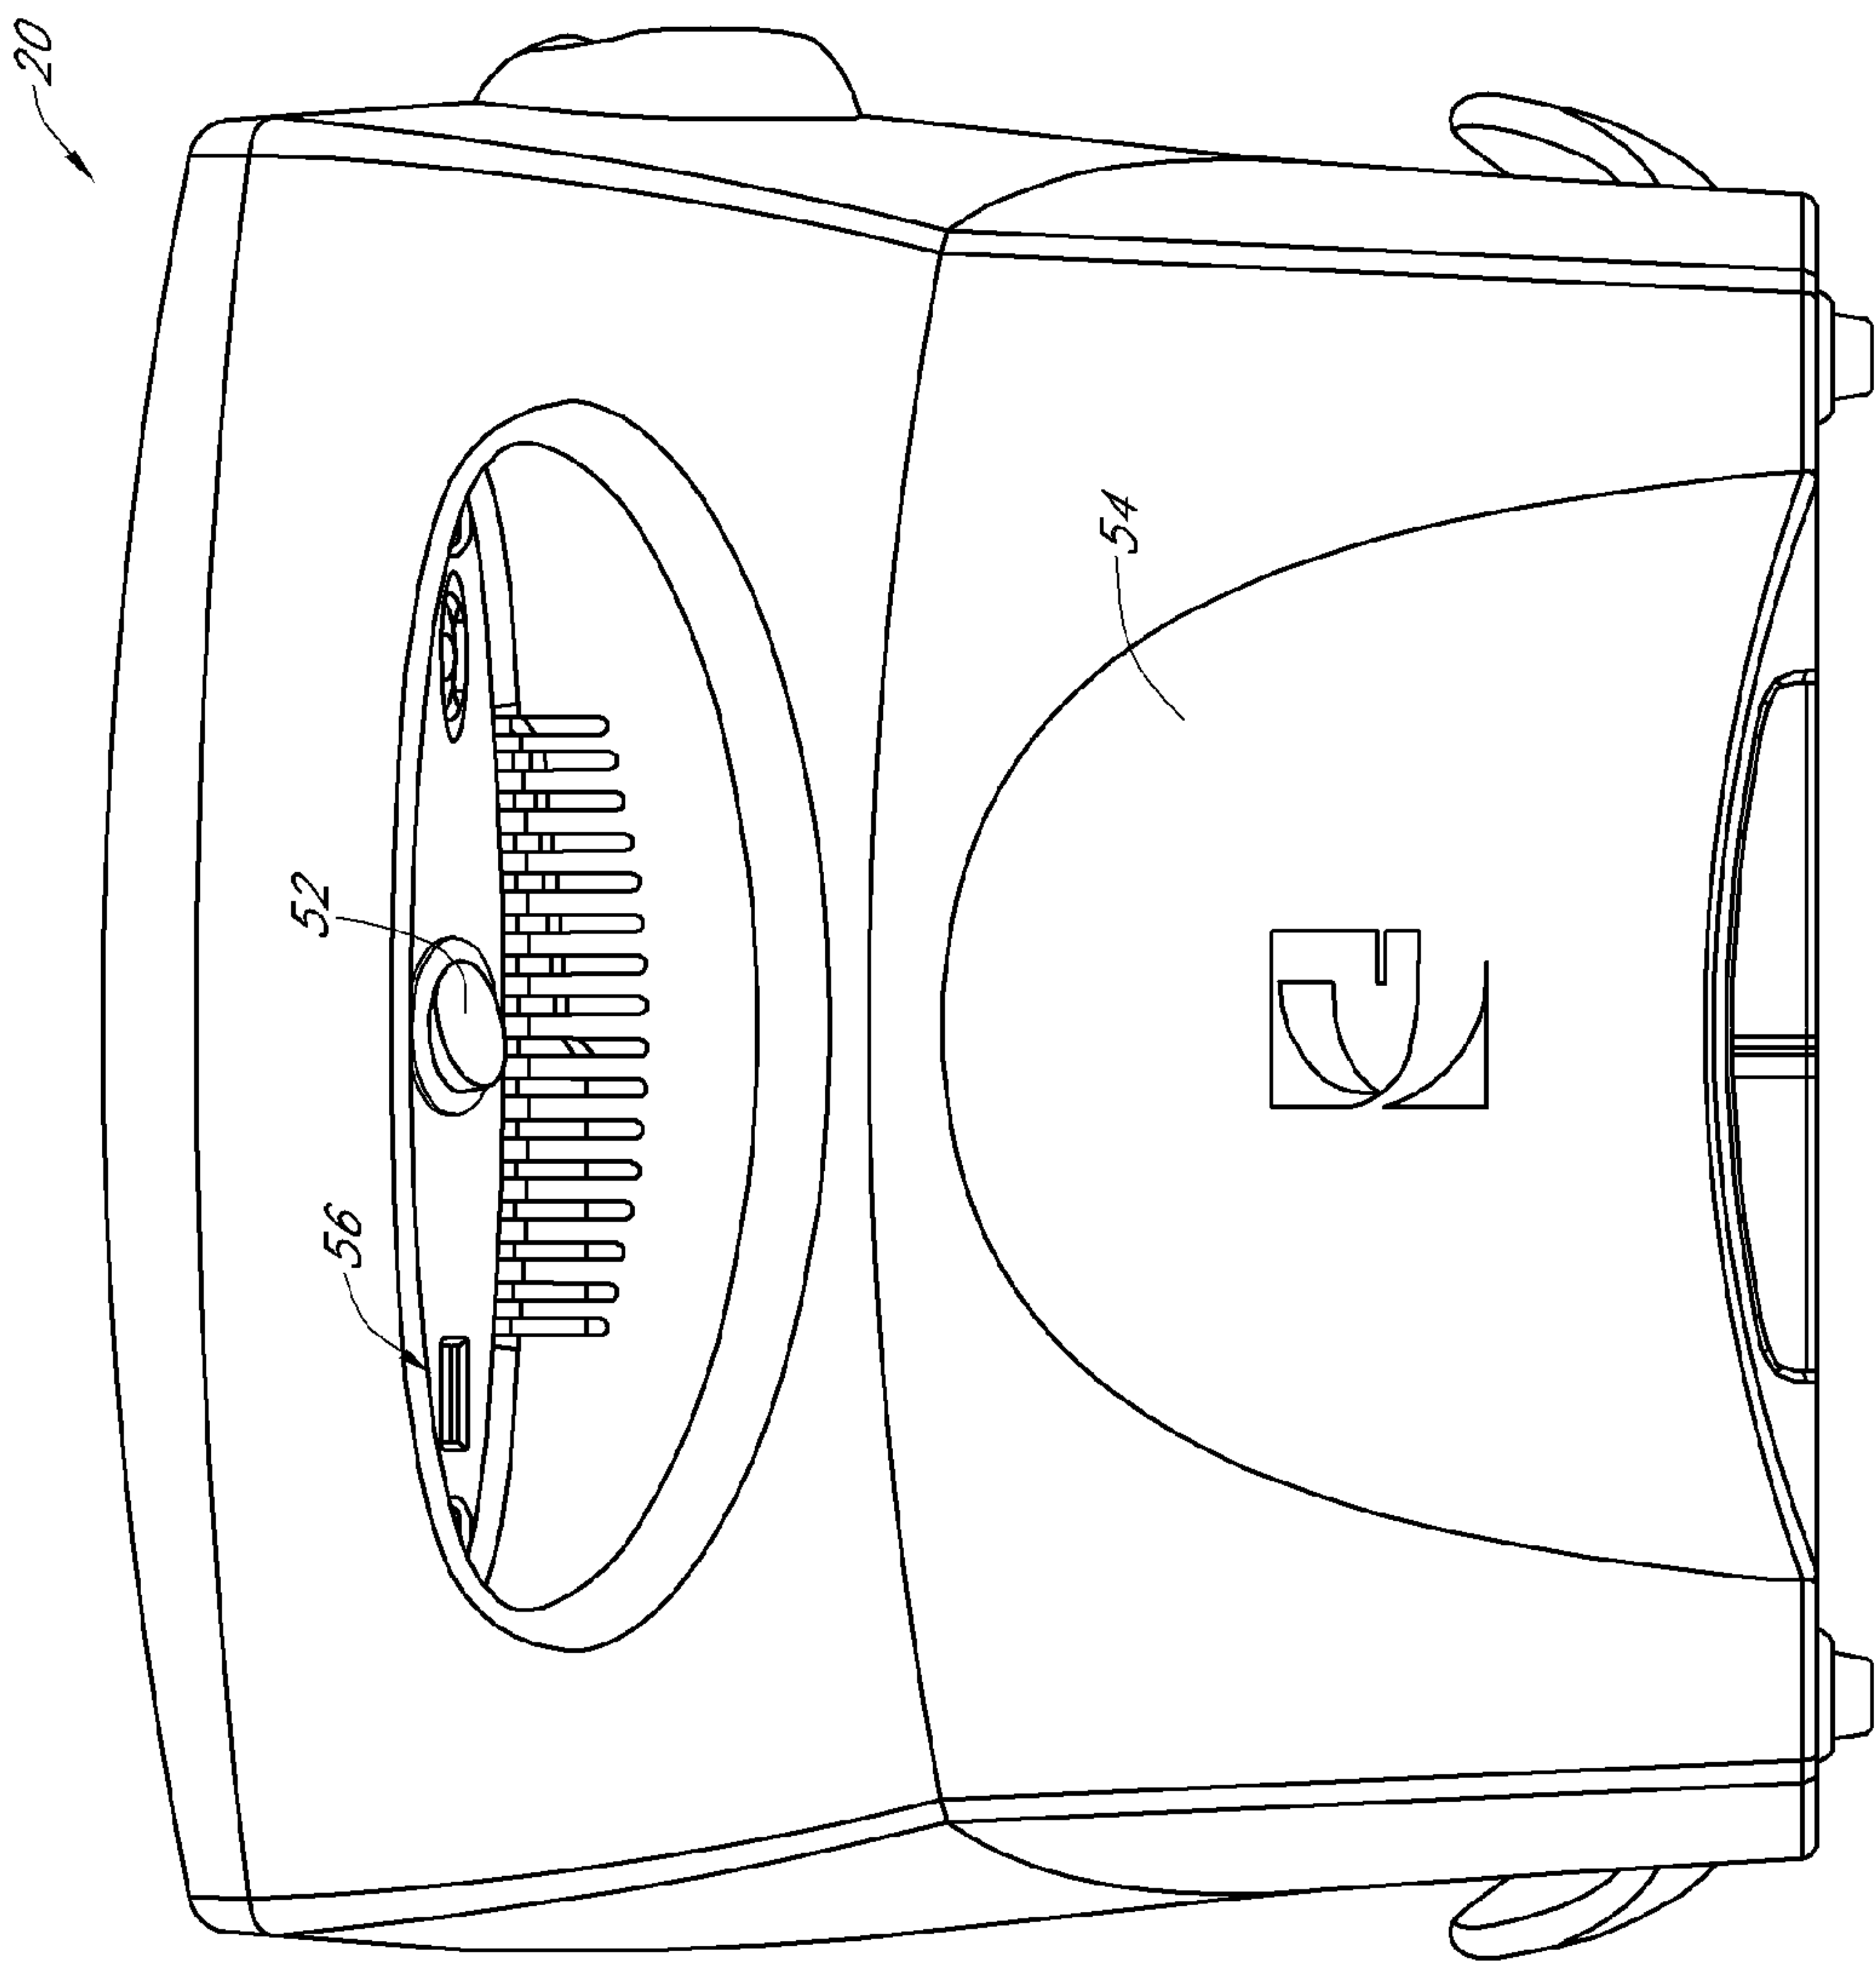


FIG. 3

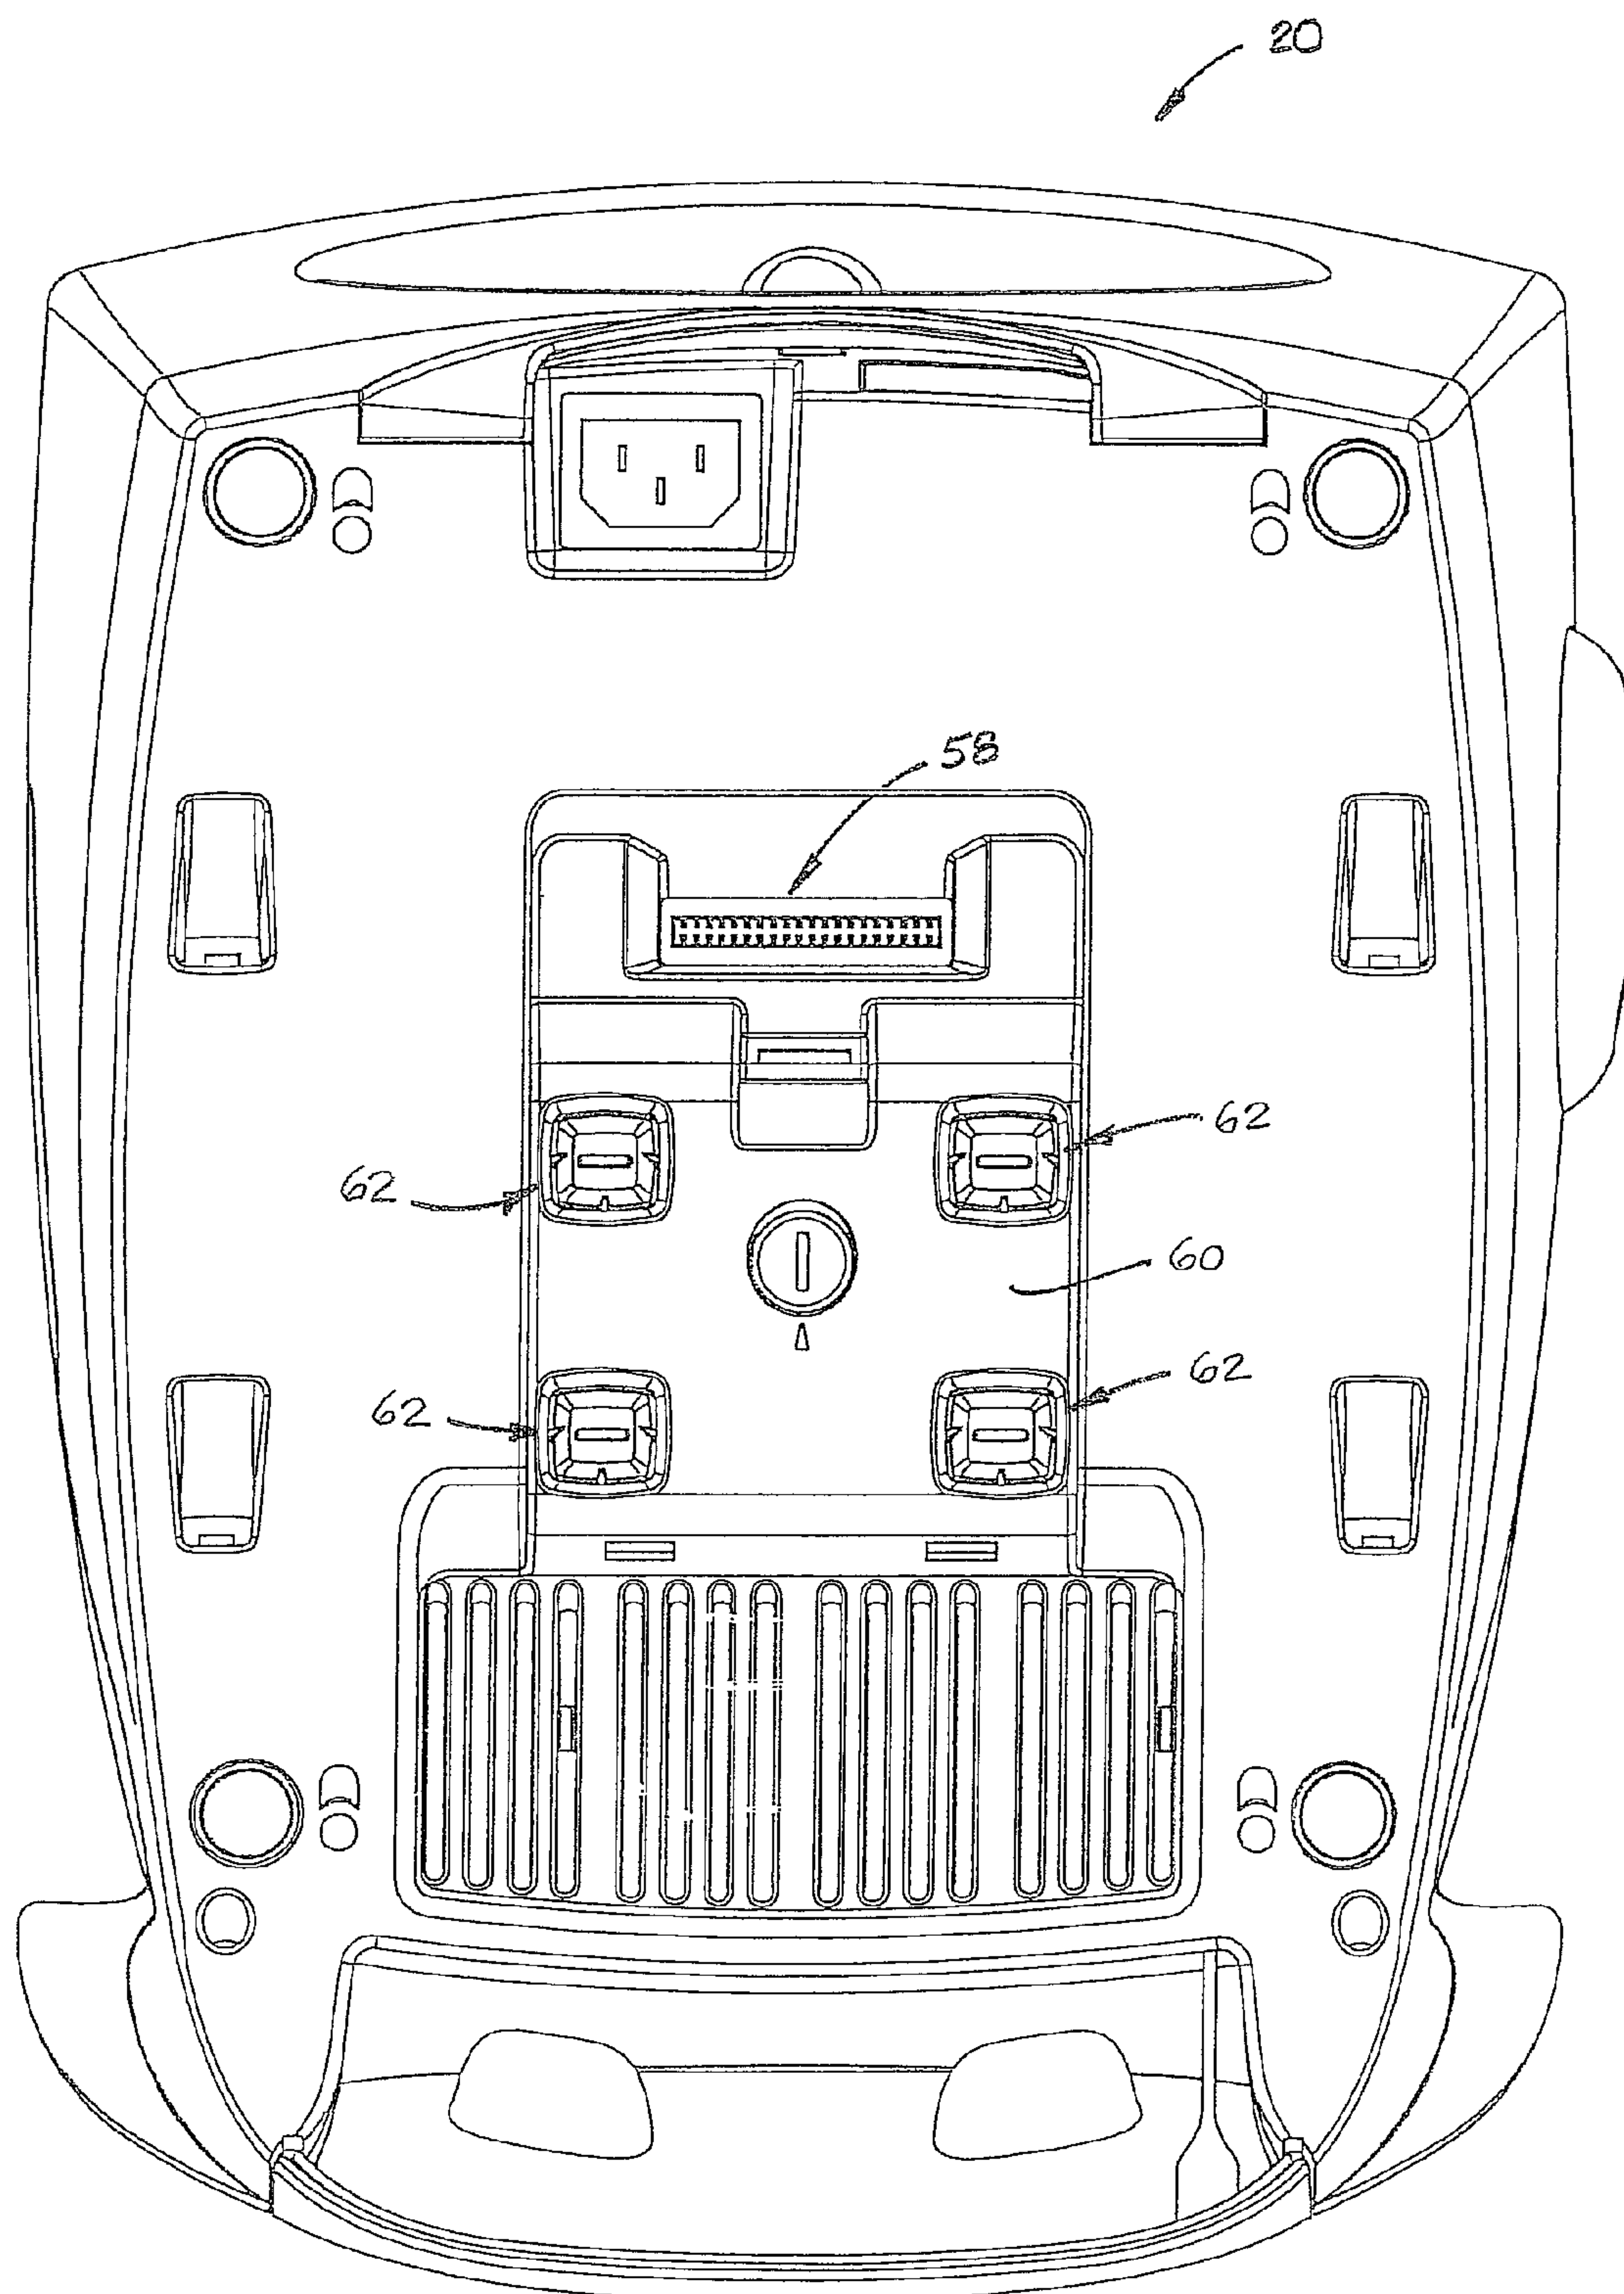


FIGURE 4

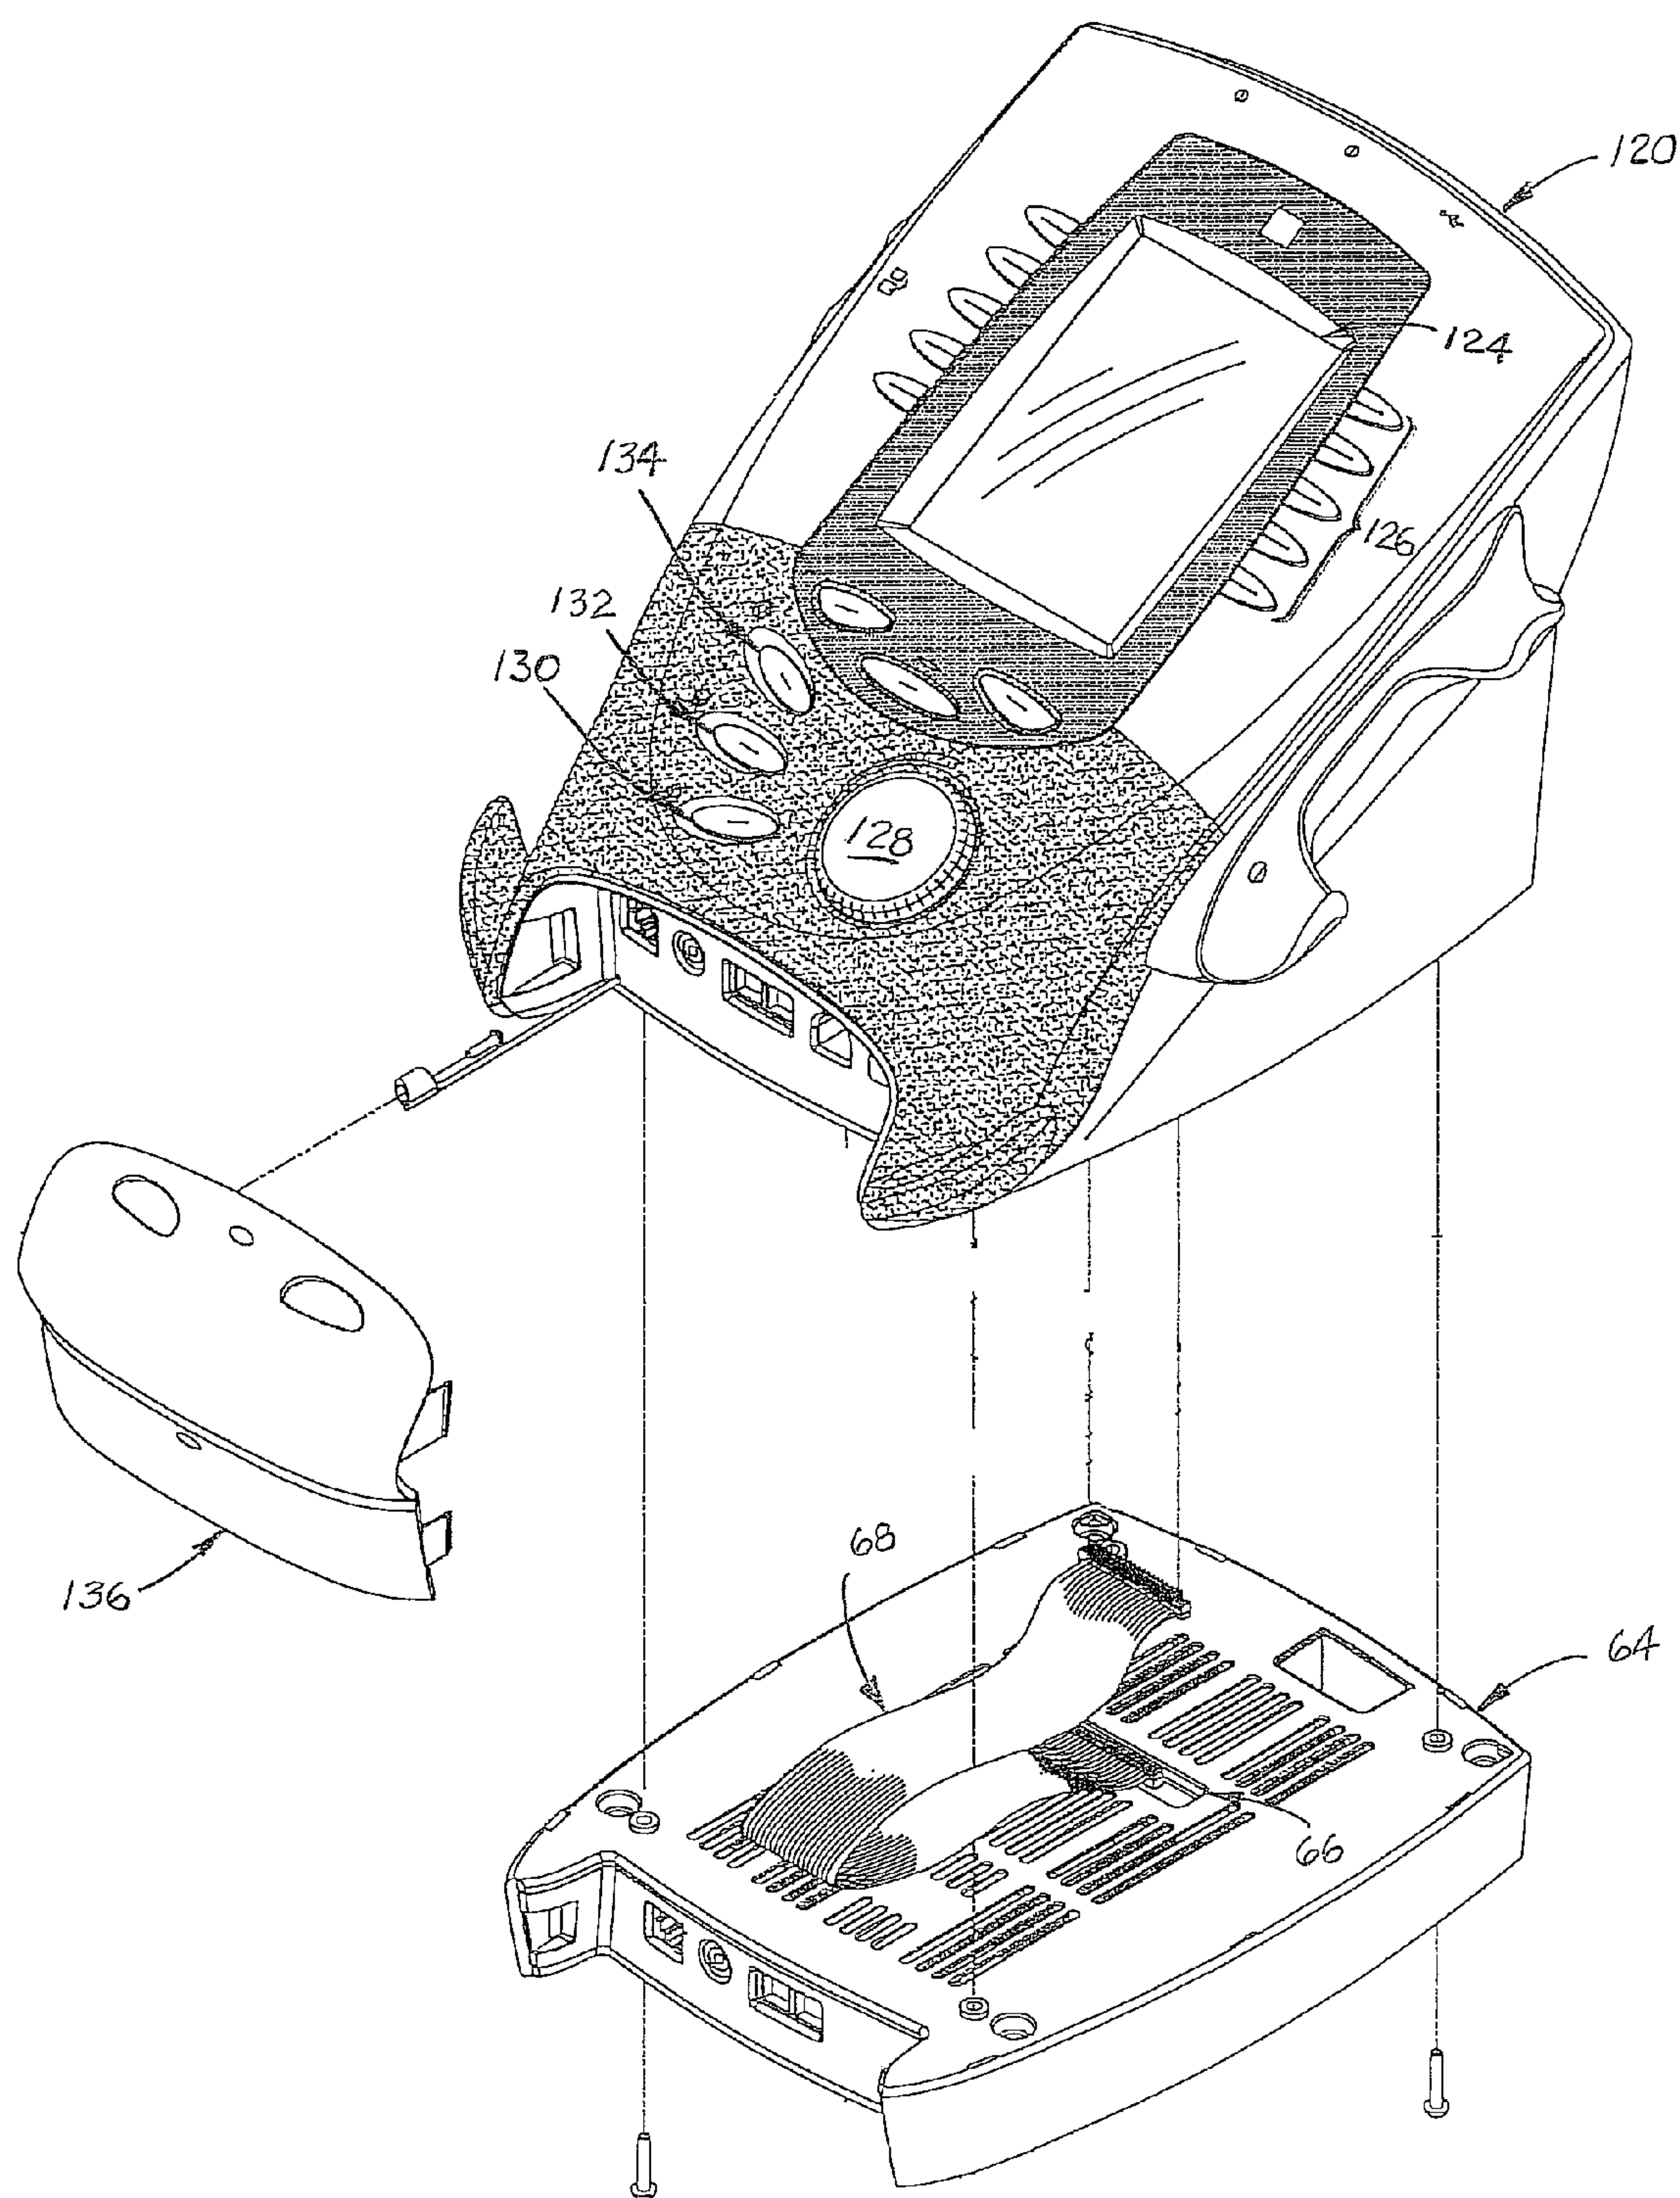


FIGURE 5

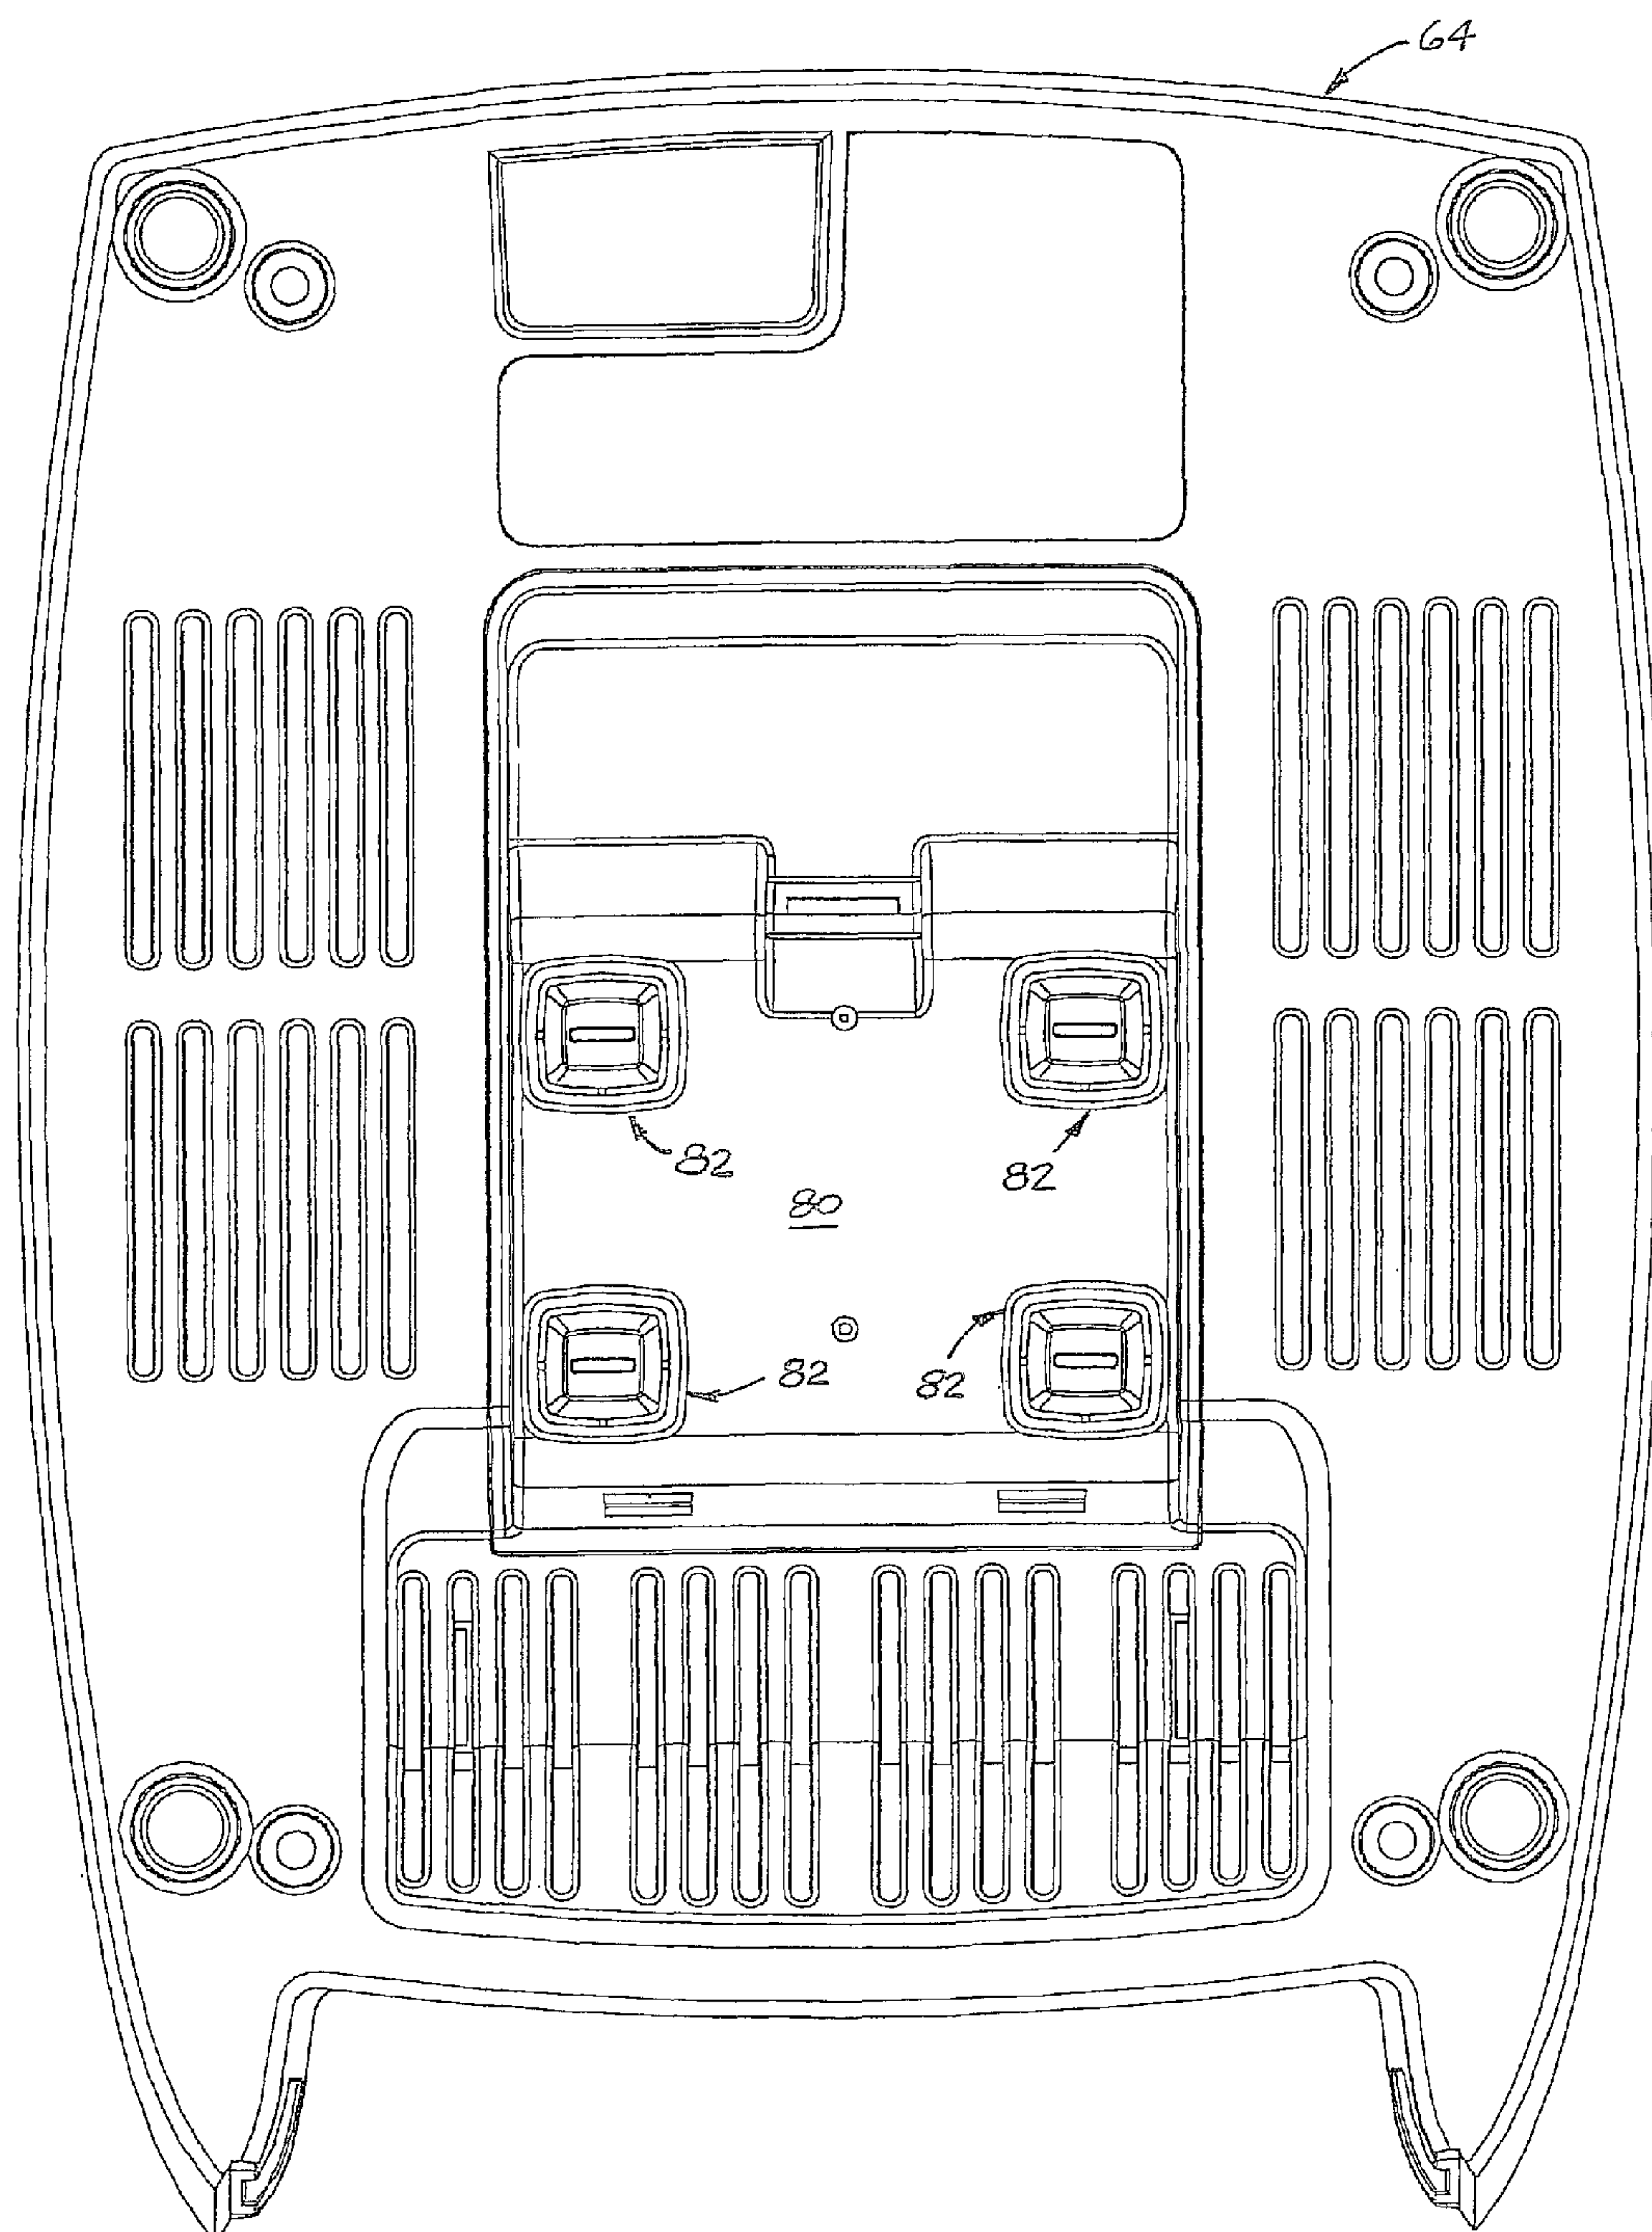


FIGURE 7

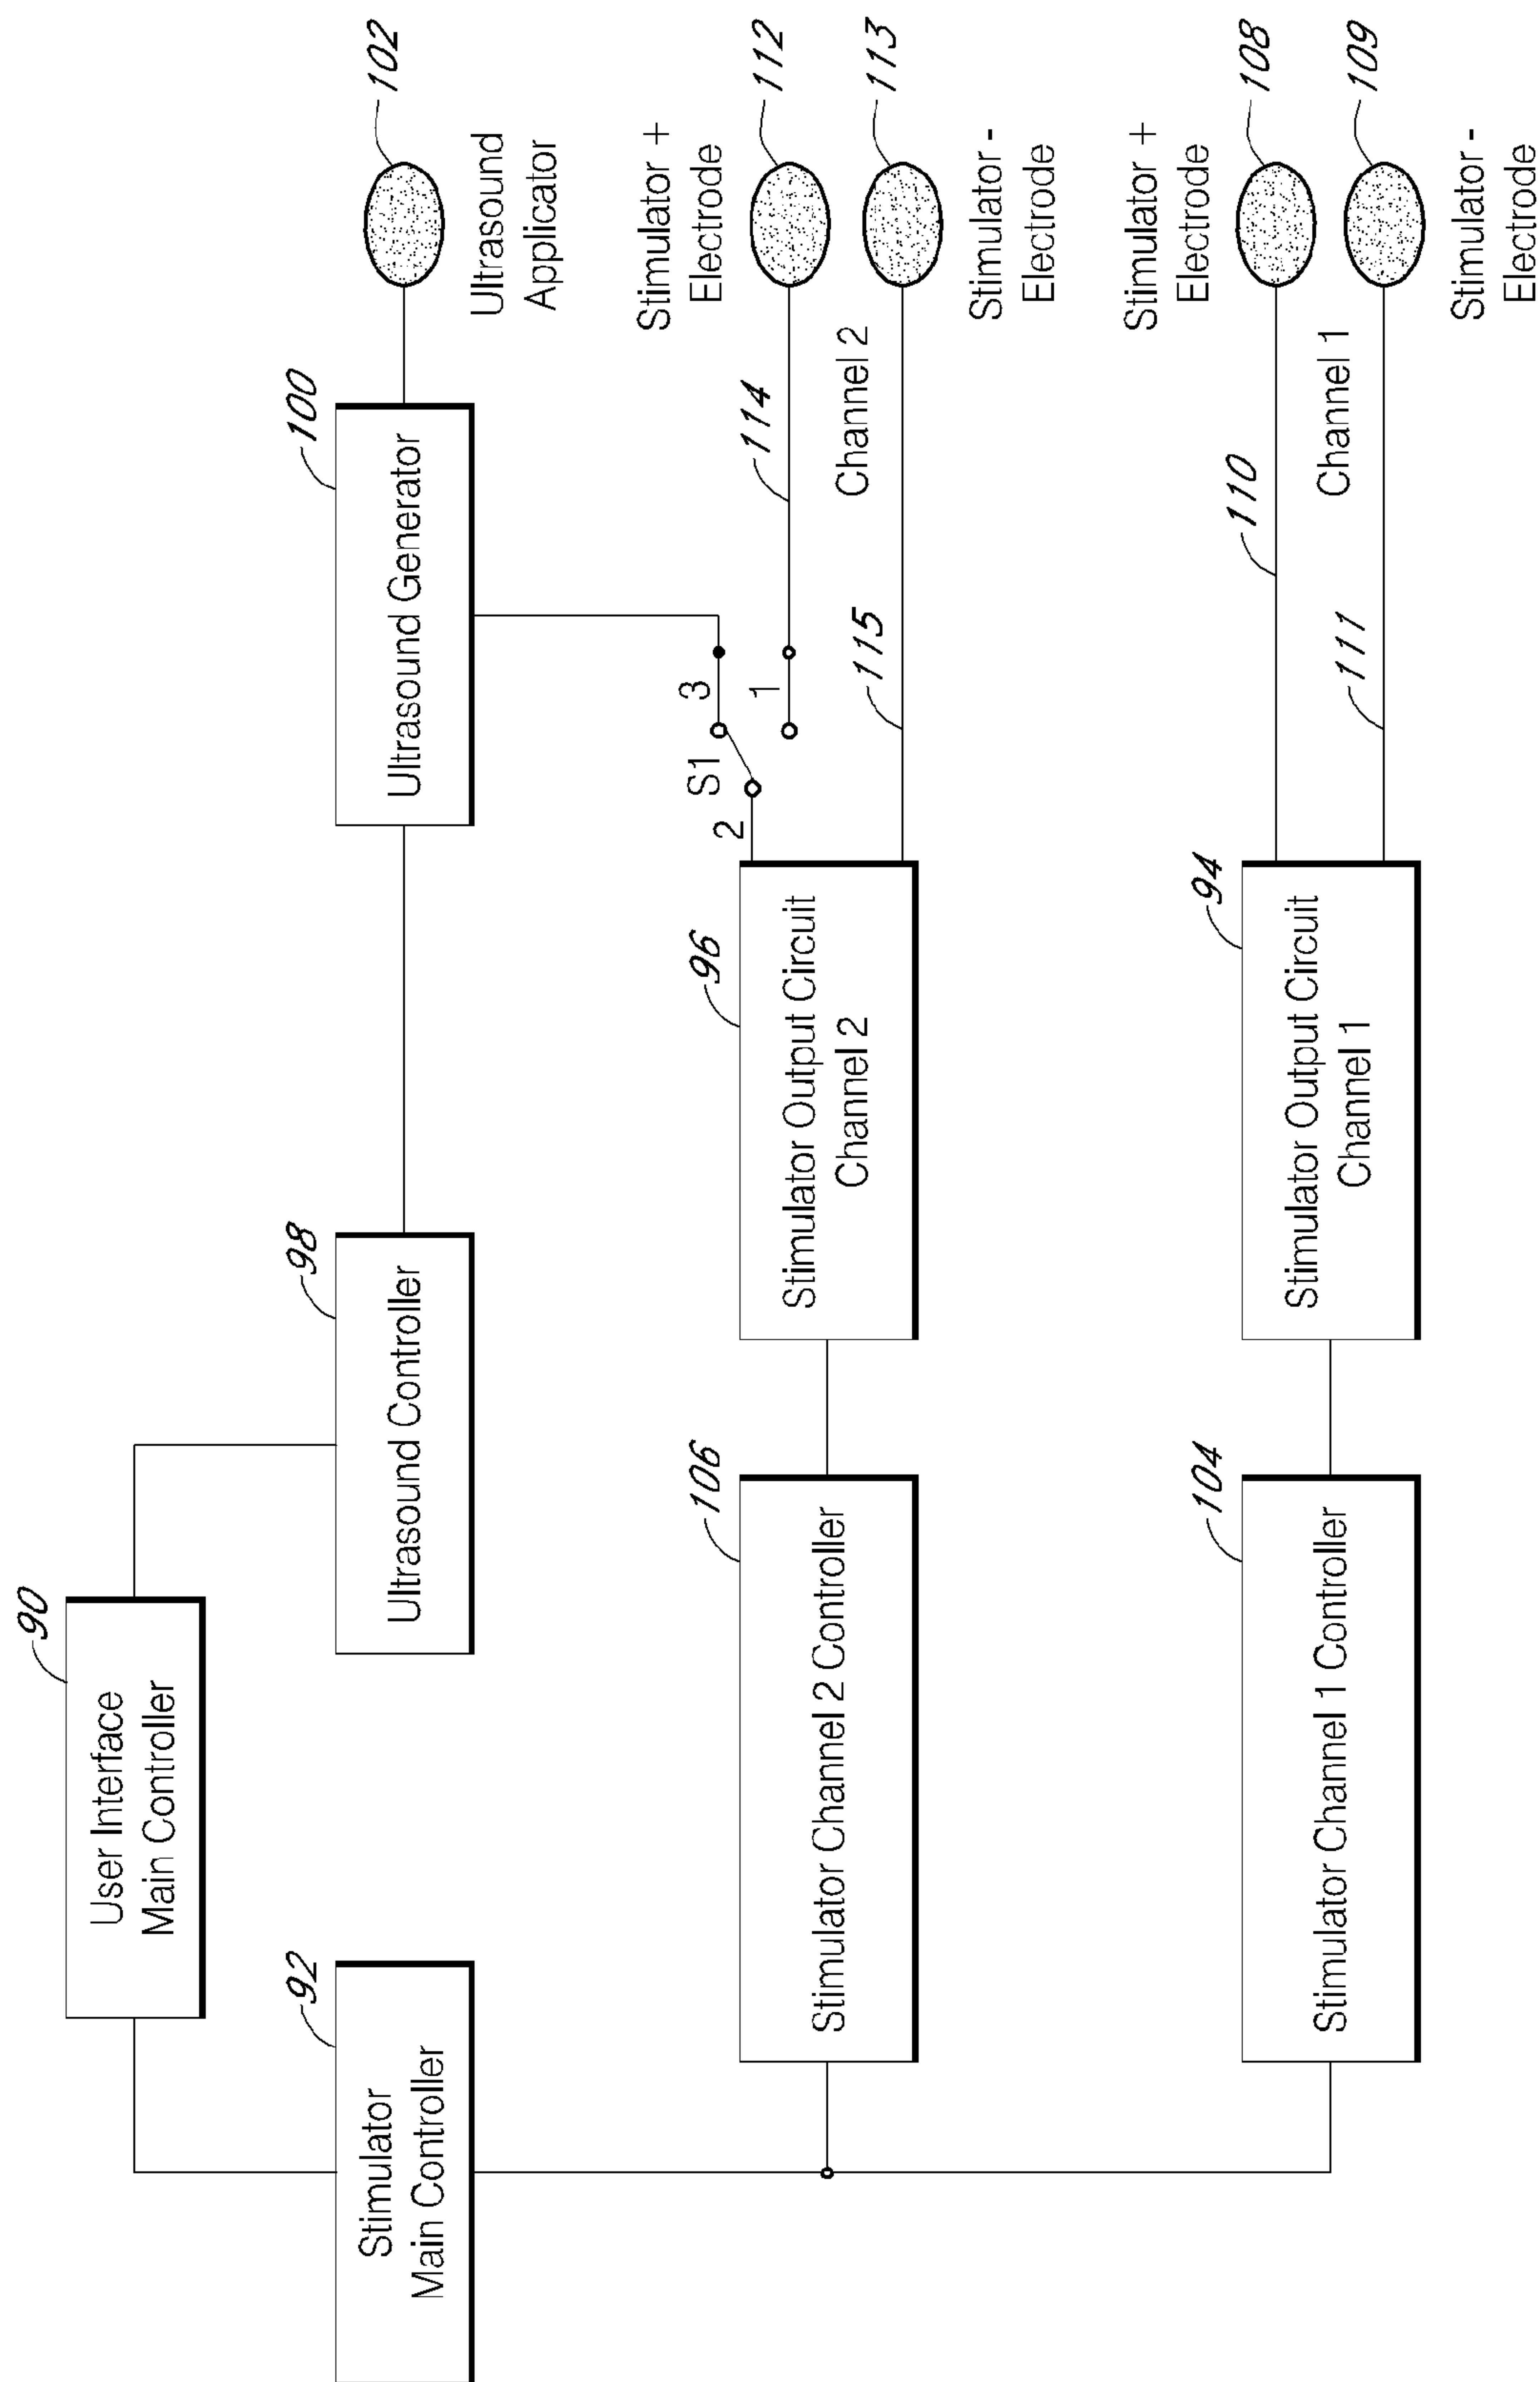


FIG. 8

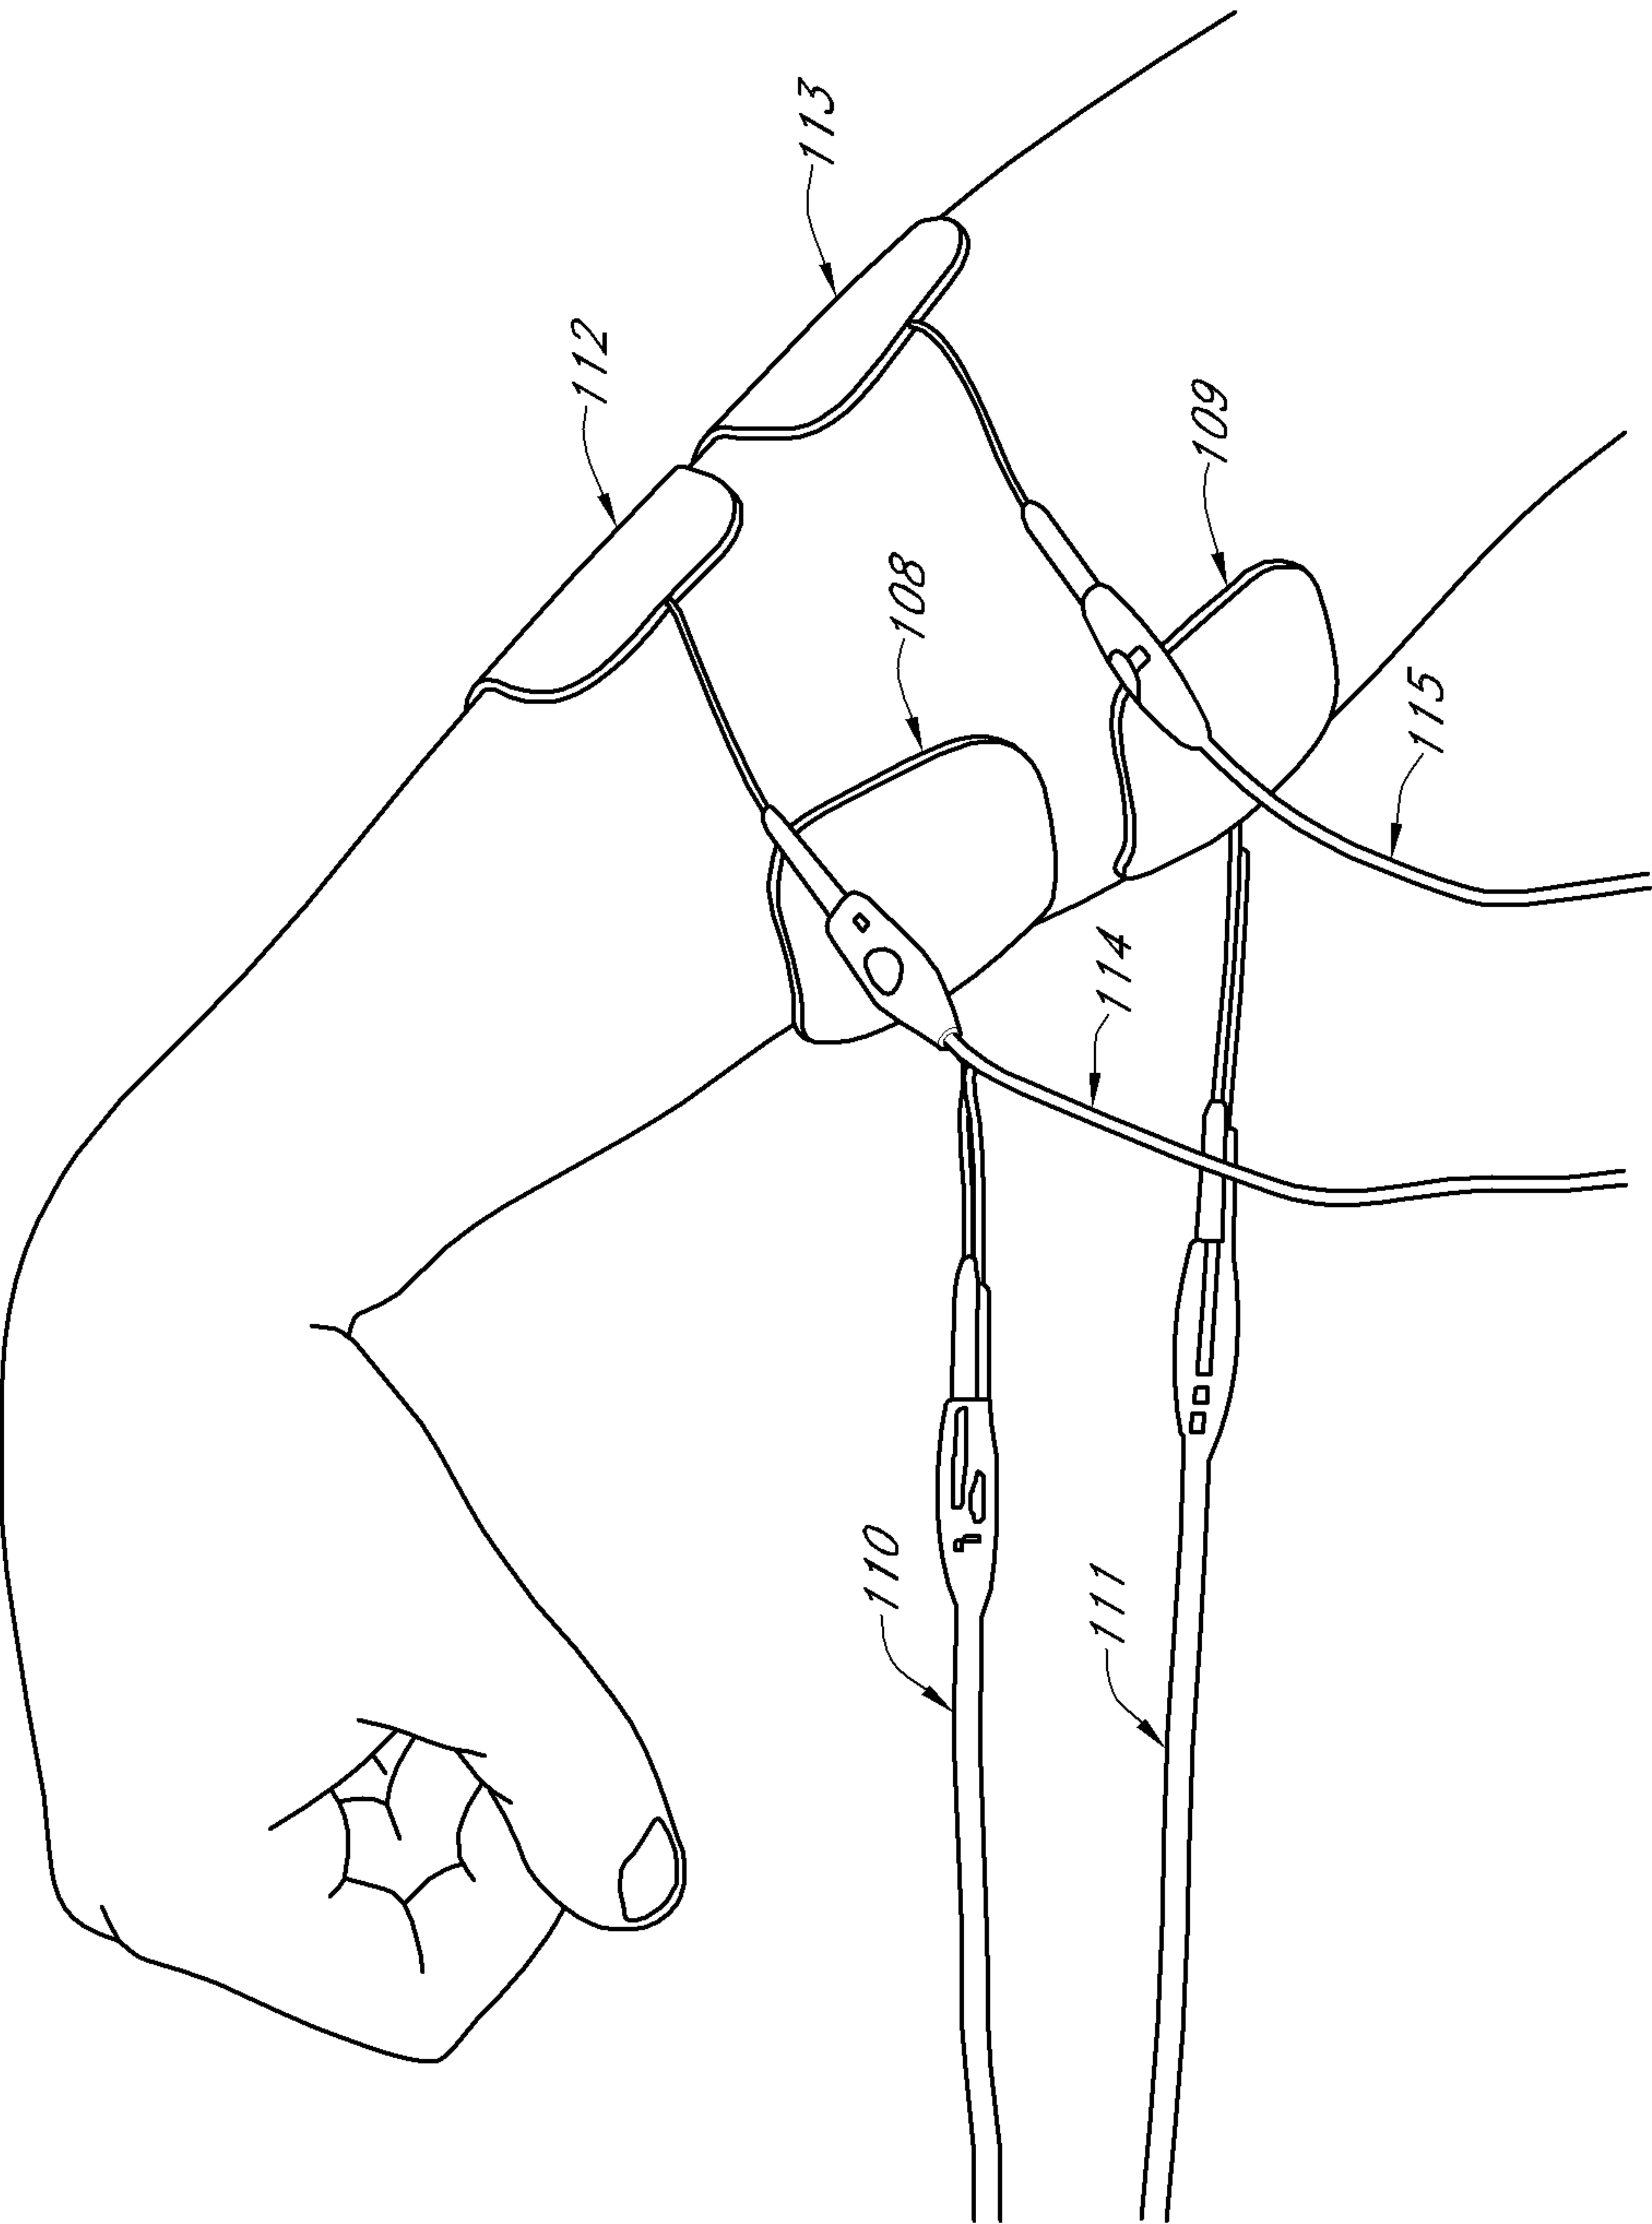


FIG. 9

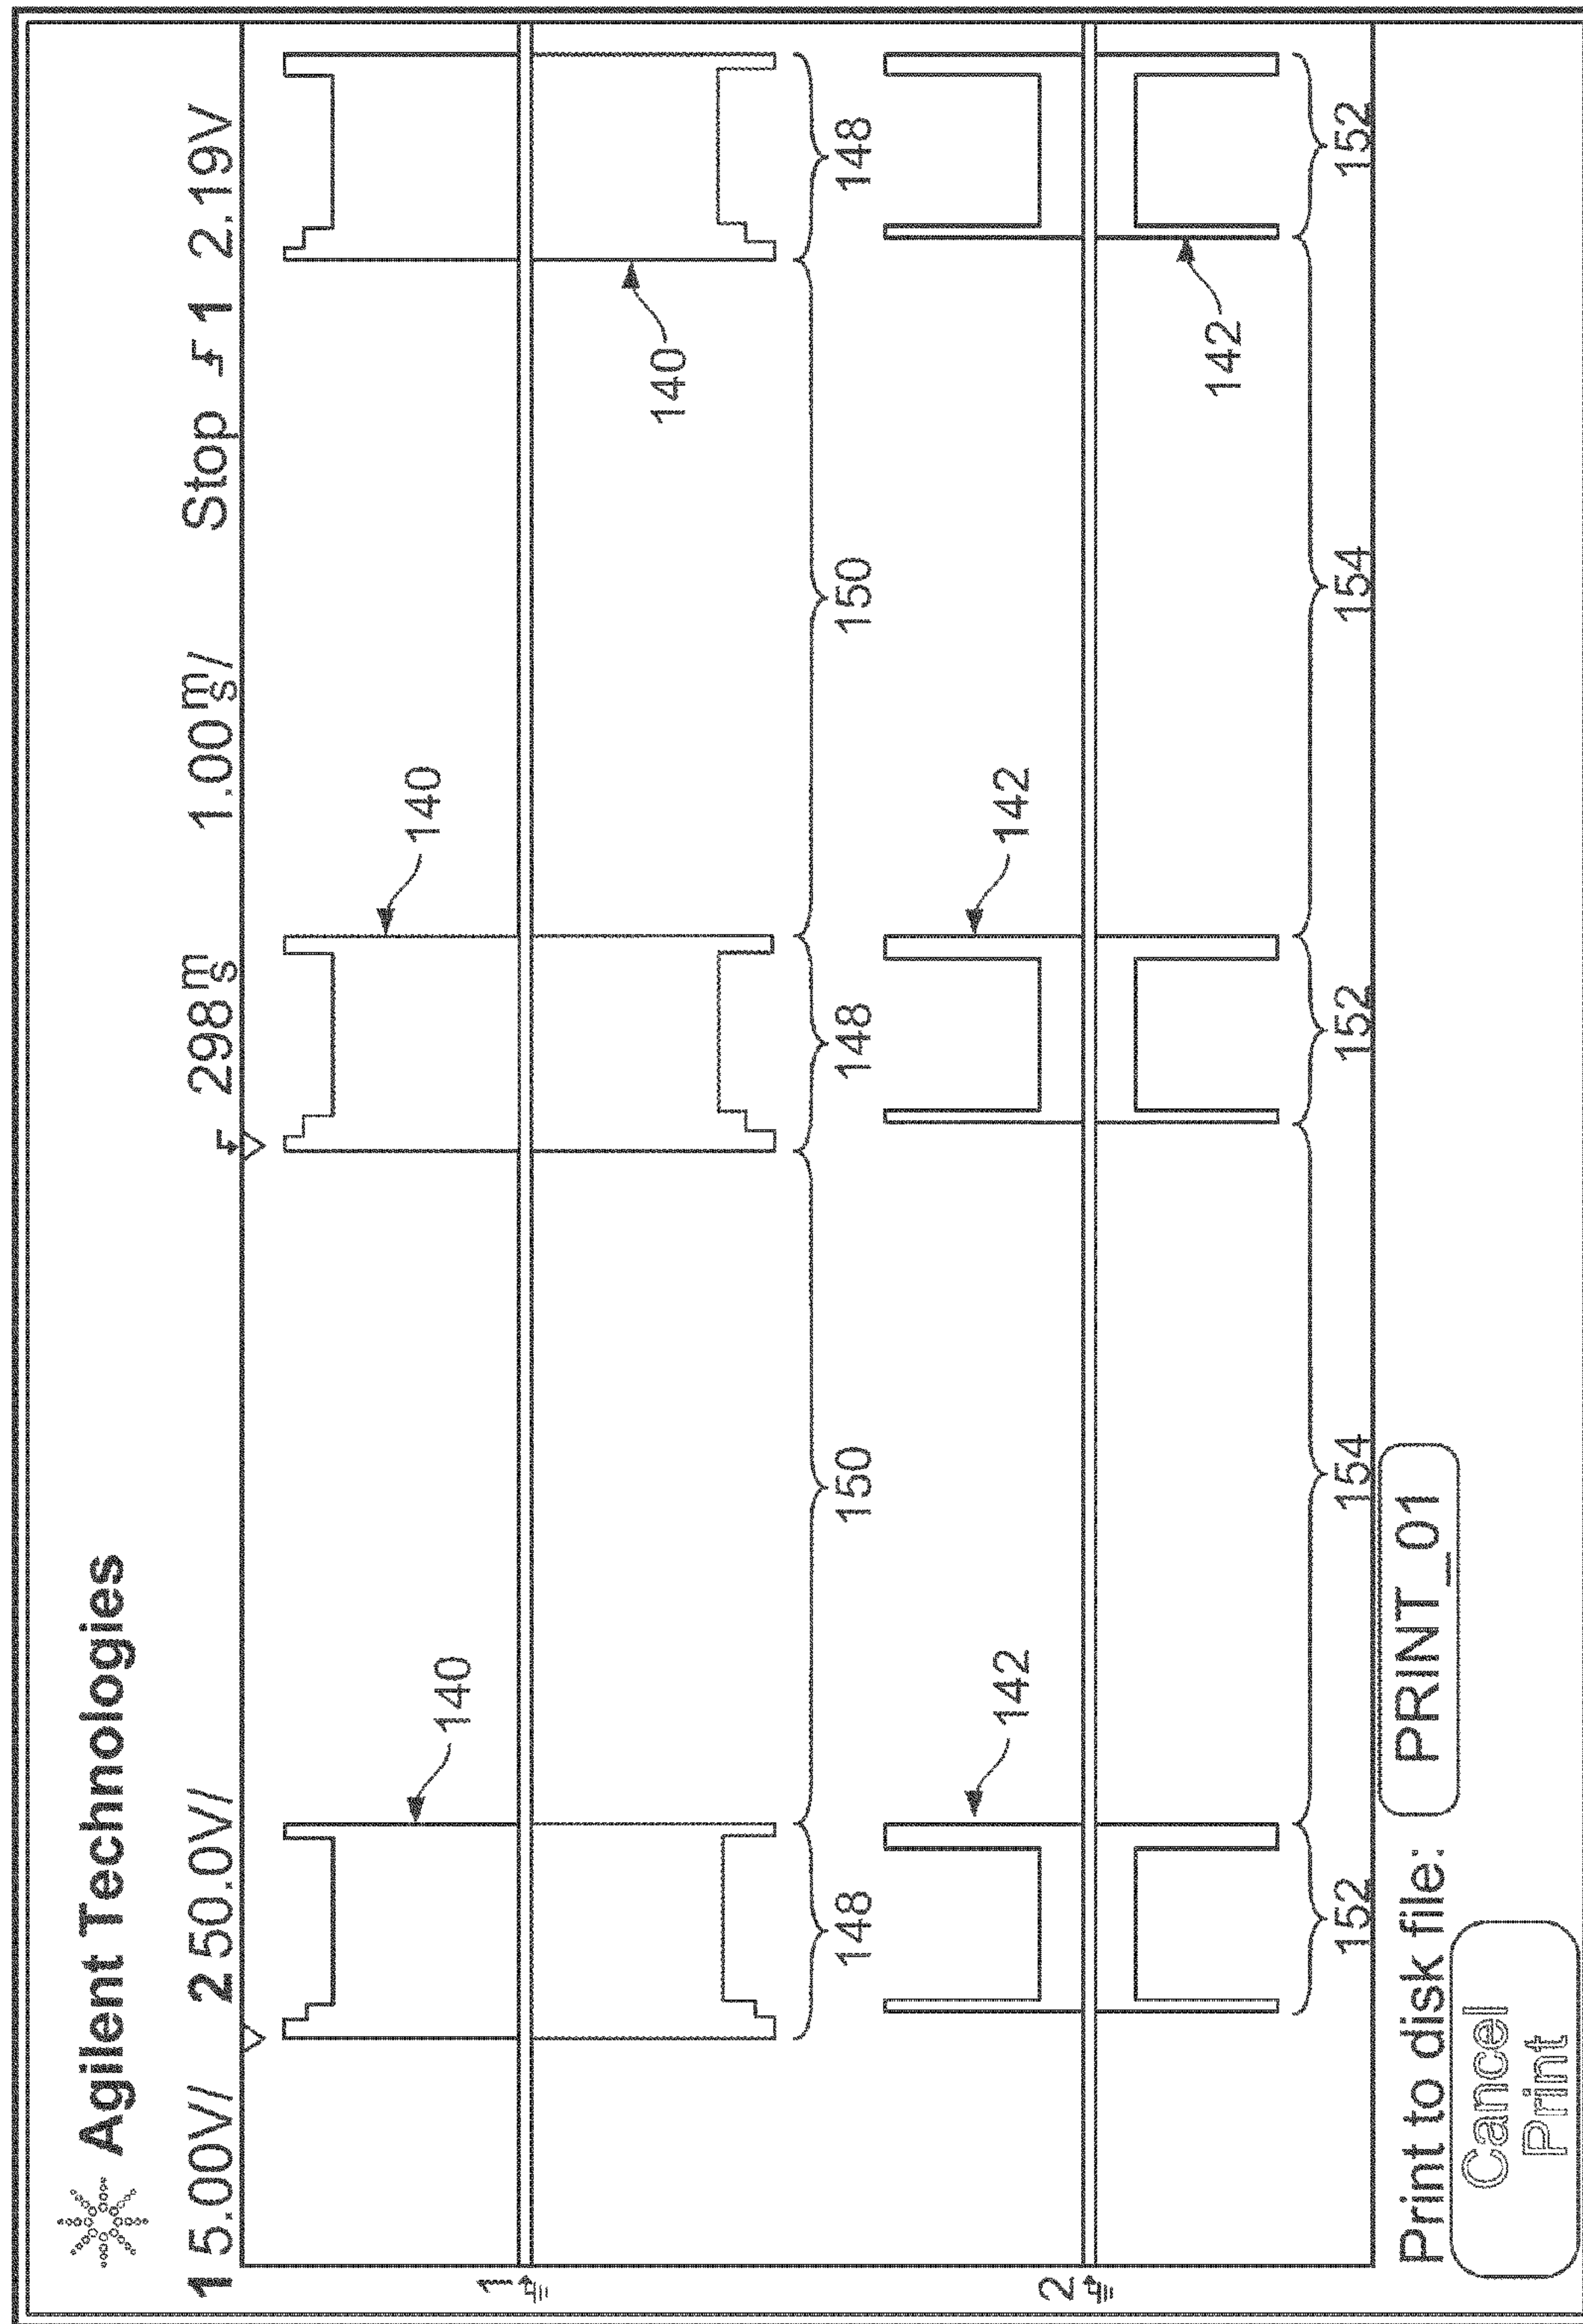


FIGURE 10

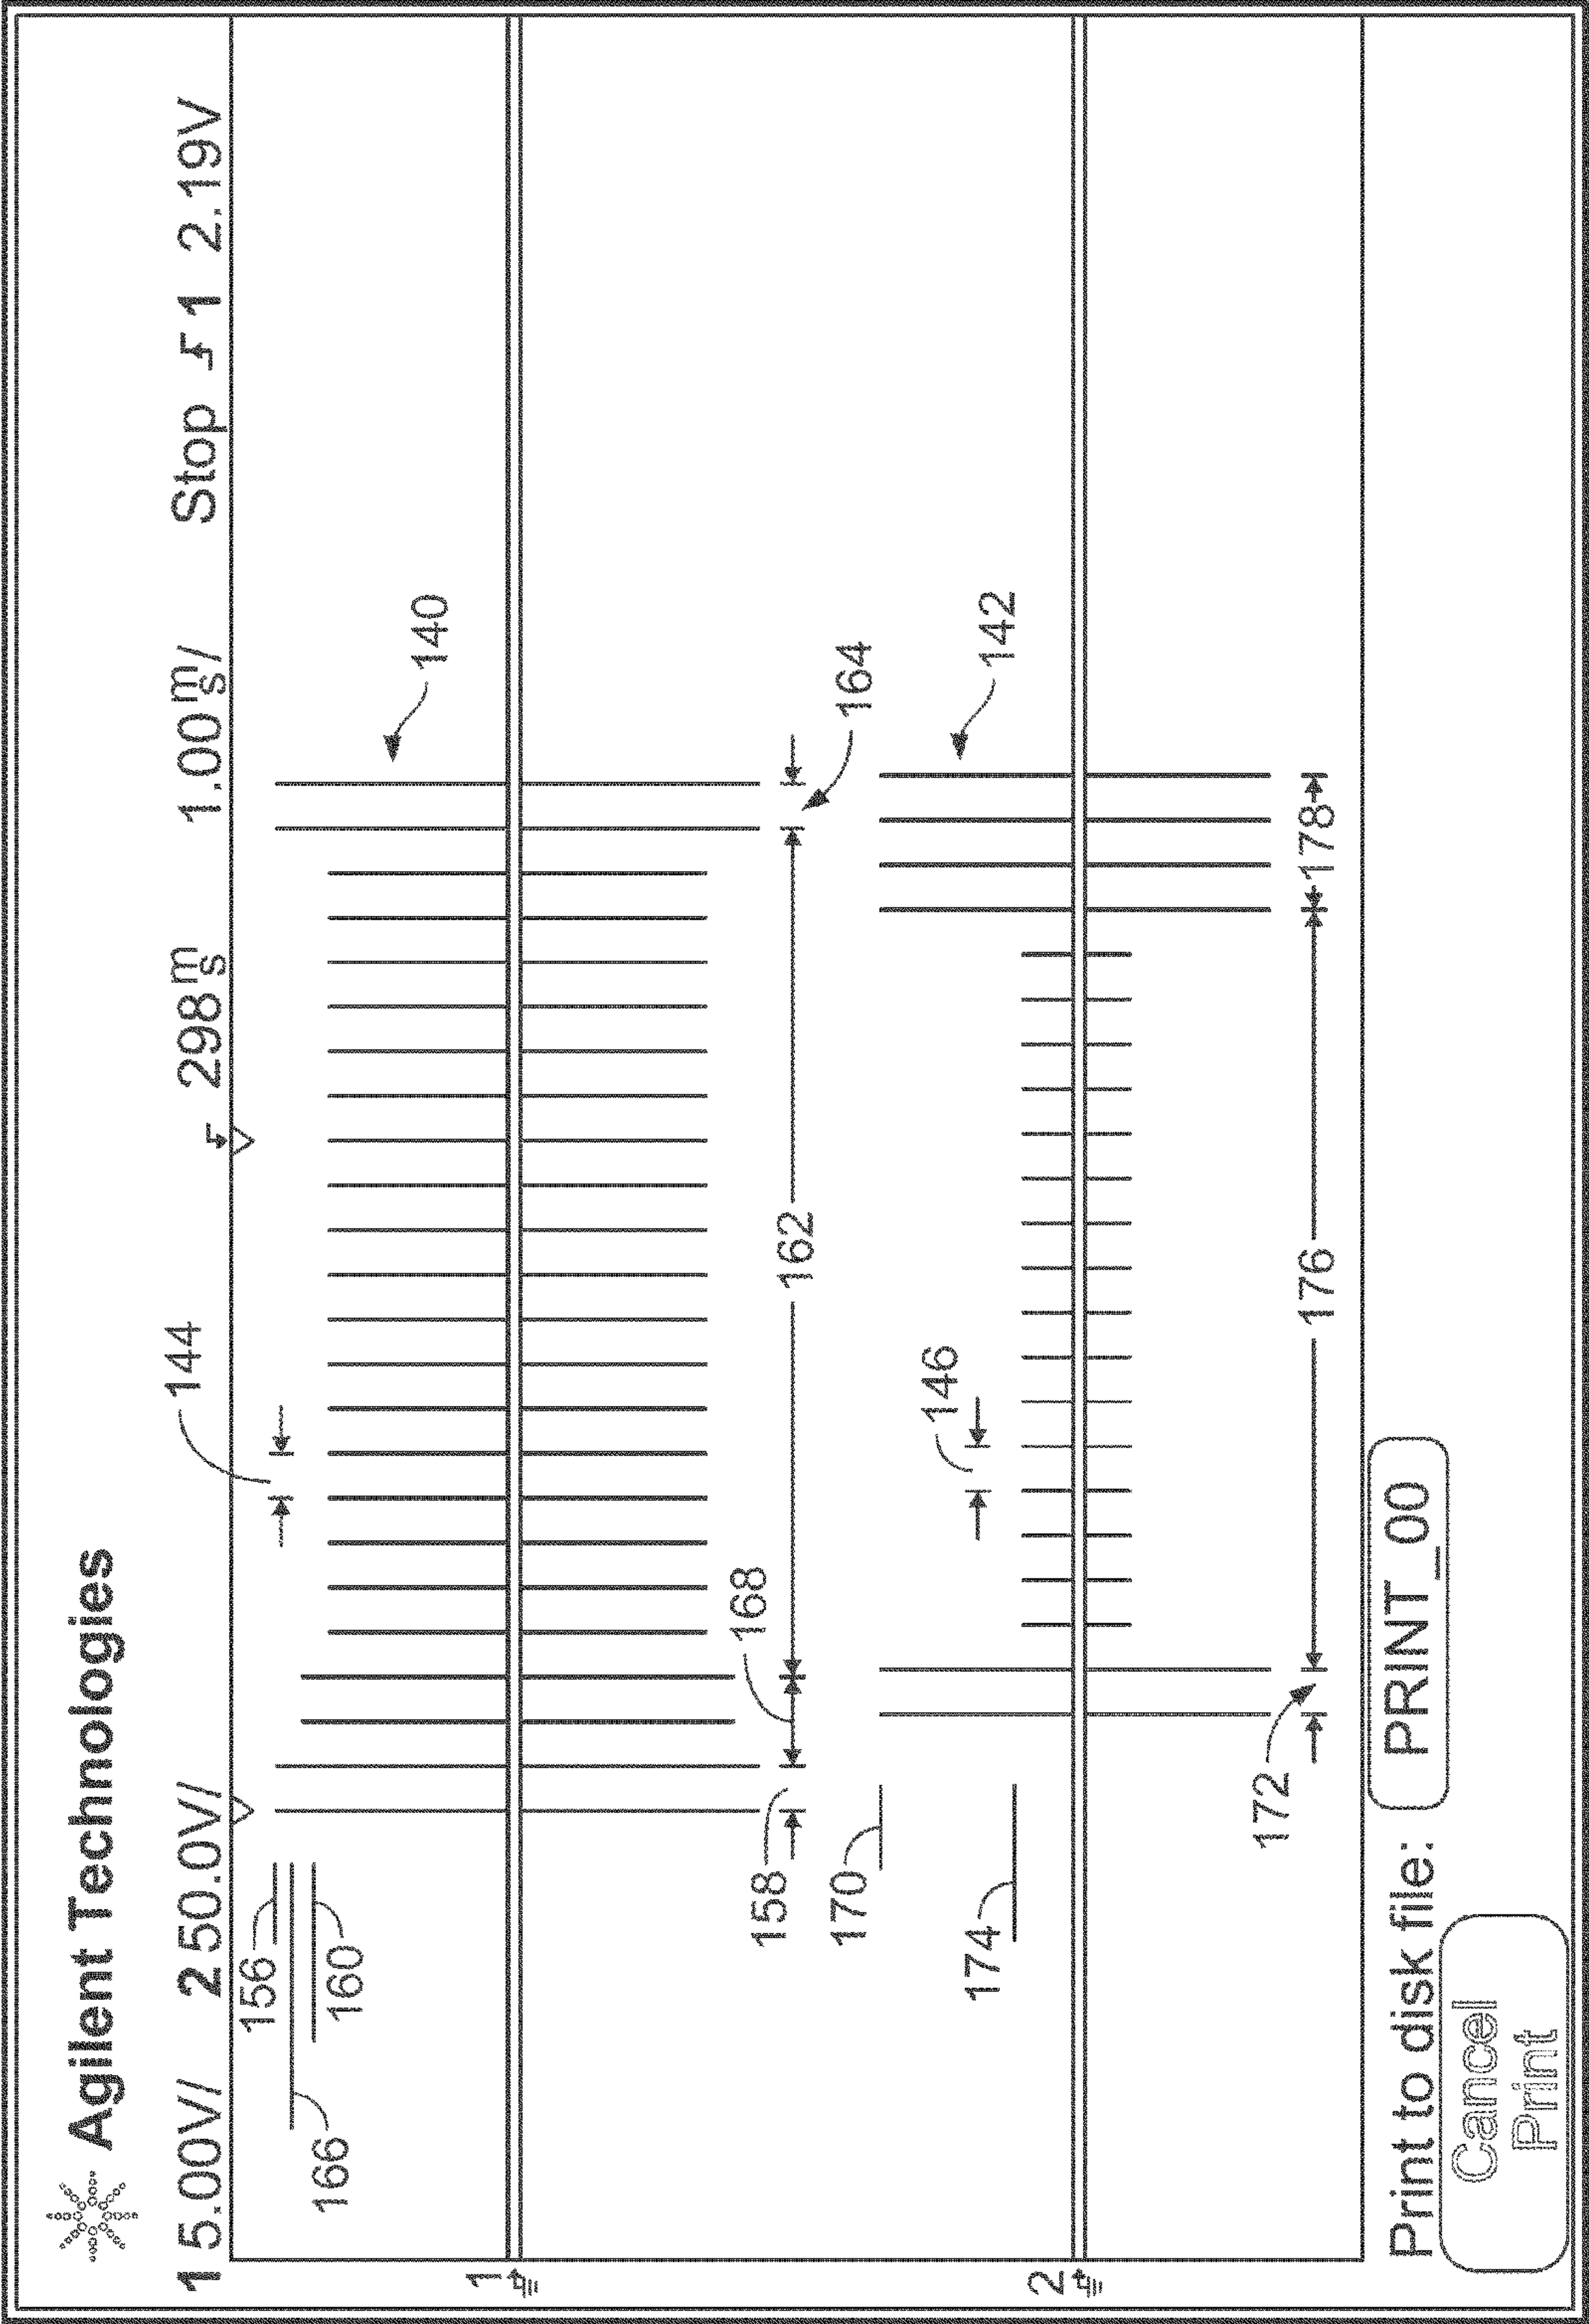


FIGURE 11

METHOD AND APPARATUS FOR APPLYING NEUROMUSCULAR ELECTRICAL STIMULATION

FIELD OF THE INVENTION

The present invention relates generally to neuromuscular electrical stimulation, and more particularly, to a method and apparatus for applying neuromuscular electrical stimulation for inducing muscle contraction in flexing, extending, adducting or abducting a limb at a joint.

EXPLANATION OF TECHNICAL TERMS

As used herein, the term "burst period" and similar terms refer to the period of time during which the neuromuscular stimulation is applied to the muscles of the patient. As used herein, the term "rest period", "rest interval" and similar terms refer to the period of time between burst periods during which the neuromuscular stimulation is not applied to the muscles of the patient.

As used herein, the terms "frequency", "pulse rate" and similar terms refer to the rate at which neuromuscular electrical stimulation pulses are delivered. The frequency is commonly expressed in hertz (Hz).

As used herein, the terms "pulse width", "pulse duration" and similar terms refer to the duration of the positive phase of the waveform.

BACKGROUND OF THE INVENTION

Neuromuscular electrical stimulation (NMES), sometimes referred to as "functional electrical stimulation" or "FES", is a technique by which muscles are induced to contract by application of electrical stimulation. NMES can be used along with exercise to strengthen an athlete's muscles, or it can be used therapeutically to strengthen and retrain muscles that have been weakened or damaged by disease or traumatic injury. NMES can also be used when voluntary motor ability is irretrievably lost, such as may arise from various forms of paralysis, to induce contractions that provide muscle benefits similar to that obtained by voluntary exercise. NMES may be distinguished from transcutaneous electrical nerve stimulation (TENS) which is used to treat pain by masking pain signals before they reach the brain.

Frequently, NMES has been applied in an attempt to activate muscles over which a patient has little or no conscious control. Thus, for example, U.S. Pat. No. 3,344,792 of Offner et al. describes a method and apparatus for applying NMES to the muscles of the lower leg to aid in walking. According to this patent, one electrode is placed on the skin over the tibialis anticus muscle and another is placed on the skin over the peroneus longus muscle. The two electrodes are then connected to a portable stimulator which is controlled by a pressure-responsive foot switch. The switch is opened when pressure is applied by the heel to the switch, and it is closed when pressure is removed. When the switch is closed, the stimulator unit applies brief pulses of current having a duration of 50 microseconds or less and an amplitude of 50 to several hundred milliamperes. The voltage required is generally on the order of 50-150 volts. As described in the Offner patent, the application of electrical stimulation in this manner not only serves as "a therapeutic method", but also serves as "a substitute for the individual's own nervous system, providing effective utilization of the individual's muscles."

U.S. Pat. No. 4,342,317 of Axelgaard describes a method and apparatus for applying neuromuscular electrical stimula-

tion to the muscles in the thorax for correction of spinal curvature deficiencies. According to this patent, a pair of specific muscle sites within the muscle group to be treated are selected, so that stimulation of the two muscle sites, on an alternating basis, will not result in any overlap of stimulation. A dual channel alternating stimulator is employed to generate alternating ON/OFF waveforms for each channel. The amplitude of the stimulating pulses is within the range of 60-80 milliamperes, and the ON/OFF times for each of the two channels are adjusted so that one muscle group starts to contract while the other starts to relax, and vice-versa.

U.S. Pat. No. 4,392,496 of Stanton describes a dual-channel neuromuscular electrical stimulator which is adapted for neuromuscular stimulation at two sites for exercising muscles to prevent disuse atrophy while minimizing fatigue. The stimulator provides, on two output channels, alternating pulsed stimulation signals which are increased in intensity at a variable rate until a fixed intensity is reached. The pulses are applied during an adjustable predetermined stimulation period and removed during an adjustable predetermined resting interval. In the preferred embodiment of the invention, the pulse rate is adjustable between 3 and 50 pulses per second.

U.S. Pat. No. 4,569,352 of Petrofsky et al. describes a feedback control system that employs a plurality of sensors and electrodes through which neuromuscular electrical stimulation is applied to enable standing and walking by paraplegic and quadriplegic persons. A programmed microprocessor produces hip movement by generating control signals for stimulation transducers which stimulate the iliopsoas and hamstring muscles. Knee flexion is produced by transducers which stimulate the quadriceps muscles, and ankle movement is produced by stimulating the gastrocnemius and tibialis muscles. The stimulation circuitry creates a series of alternating pulses at a frequency of 50 Hz.

U.S. Pat. No. 4,586,495 of Petrofsky describes a method and apparatus for stimulating the muscles of a patient who has suffered a spinal cord injury during the period following the injury and prior to the time when stimulated dynamic exercise may be commenced according to the method and apparatus of U.S. Pat. No. 4,569,352. The apparatus of the '495 patent includes a leg brace which maintains the knee and ankle at predetermined angles. Electrodes are applied to the muscles of the braced leg over the agonist and antagonist muscles for bending the leg about the knee and ankle joints. The hamstring and quadriceps muscles function as agonist and antagonist muscles, respectively, for the knee joint and the tibialis anterior and gastrocnemius muscles function as agonist and antagonist muscles, respectively, for the ankle joint. In the preferred embodiment of the invention, the quadriceps muscles are stimulated for approximately four seconds to cause the muscles to attempt extension against the restraint of the brace. Thereafter, the quadriceps muscles are rested and the hamstring muscles are stimulated for four seconds to cause the muscles to attempt to bend the knee against the restraint of the brace. Then both sets of muscles are rested for four seconds, and the sequence is repeated. After the hamstring and quadriceps muscles have been exercised, the electrodes are placed on the tibialis anterior and gastrocnemius muscles and a similar stimulation sequence is begun for these muscles. A pair of load cells on the leg brace provide feedback signals to a computer which controls the application of the electrical stimulation signals. As the muscles tire with exertion, the computer increases the stimulation level until a maximum value of 50 volts is reached. Each stimulation signal comprises a series of pulses having a pulse width of about 300 microseconds and a frequency of 40 pulses/second.

As mentioned above, NMES can be used along with exercise to strengthen an athlete's muscles, or it can be used therapeutically to strengthen and retrain muscles that have been weakened or damaged by disease or traumatic injury. Thus, for example, U.S. Pat. No. 4,622,973 of Agarwala describes a clinical device which may be used to establish an NMES regimen, as well as a portable device which is programmable by the clinical device and which automatically reproduces the NMES regimen which was established in the clinical device.

U.S. Pat. No. 4,996,987 of Petrofsky describes a method and apparatus for applying electrical stimulation to induce work-producing contraction of the muscles. According to this patent, the stimulation of work-producing contraction of muscles in patients with little or no nerve damage causes unacceptable pain. Consequently, the method of the invention includes applying a high-frequency, low-amplitude desensitizing current to the muscle to be stimulated prior to applying a low-frequency, high-amplitude stimulating current which is continuous with the desensitizing current. The stimulating current is applied as the desensitizing current is terminated, and the two currents are alternately applied so that no abrupt discontinuity occurs between the currents. Preferably, the stimulating current is a "camel-back" biphasic signal having three segments, the first and third of which are of opposite polarity to the second. The first and third segments are substantially identical in duration and magnitude, and the second has a duration equal to the sum of the durations of the first and third segments and a magnitude that is equal to and of opposite polarity to either the first or the third segment.

U.S. Pat. No. 5,562,718 of Palermo describes a device for use in applying NMES in a series of electrical pulses in the form of sequential pulse patterns, or dual or triple overlapping pulse patterns. These electrical pulse patterns are applied through a first channel by electrodes that are attached to the skin over an agonist muscle and through a second channel by electrodes that are attached to the skin over the corresponding antagonist muscle. The timing of the sequential or overlapping pulse train patterns is reportedly selected to take advantage of central nervous system inhibition and facilitation by repetitive cycling of the pulse trains to emulate reciprocating limb speeds ranging from slow gentle arm or leg movements to the fastest running patterns. The commercial embodiment of the Palermo device, marketed by Accelerated Care Plus of Reno, Nev., employs electrodes applied to the agonist and antagonist muscles to generate overlapping pulse patterns that serve to contract these muscles. According to literature published by Accelerated Care Plus, a first pulse pattern is applied through a first channel to the agonist muscle in a first burst period of approximately 75 msec., followed by a first rest interval of about 50 msec. and a second pulse pattern in a second burst period of about 50 msec. A third pulse pattern is then delivered to the antagonist muscle through the second channel in a third burst period of about 75 msec., which begins approximately 55 msec. after the beginning of the first burst period (of the first channel) and continues through the first rest interval (of the first channel) and for about 10 msec. into the second burst period.

U.S. Pat. No. 5,980,435 of Joutras et al. describes a method and apparatus for therapeutic use of a jointed brace. According to this patent, the brace is attached to a jointed limb and provides controlled resistance to movement of the limb about the joint. The brace may be used in conjunction with a neuromuscular stimulation device, and it may be programmed to resist the movement of stronger, or antagonistic, muscles against weaker, or agonistic, muscles. However, there is no force applied by the equipment to the user in the absence of an

attempt to move a limb about a joint. The force applied by the equipment is only a force of reaction.

U.S. Pat. No. 6,845,271 of Fang et al. describes a method and apparatus for treatment of shoulder dysfunction using neuromuscular electrical stimulation applied through intramuscular electrodes. Preferably, the method involves asynchronous stimulation of more than one muscle group, such as a first muscle group being the supraspinatus in combination with the middle deltoid and a second muscle group being the trapezius in combination with the posterior deltoid. This asynchronous stimulation involves intermittent periods of stimulation and rest, with one muscle group being subjected to stimulation while the other is resting.

Although it is known to apply NMES to the agonist and corresponding antagonist muscles in certain pulse patterns, the inventors have developed a method and apparatus for generating NMES pulses in patterns that appear to more accurately simulate natural movement of a limb about a joint.

SUMMARY OF THE INVENTION

The invention comprises a method and apparatus for applying neuromuscular electrical stimulation to an agonist/antagonist muscle pair to move a limb about a joint. According to this method, a device is provided for generating a first pattern of neuromuscular electrical stimulation pulses for output through a first channel to a first pair of electrodes and for generating a second pattern of neuromuscular stimulation pulses for output through a second channel to a second pair of electrodes. A first pair of electrodes is provided in operative connection to the first channel of the device, and a second pair of electrodes is provided in operative connection to the second channel of the device. The first pair of electrodes is attached to the agonist muscle of the agonist/antagonist muscle pair, and the second pair of electrodes is attached to the antagonist muscle of the muscle pair. A first pattern of electrical stimulation pulses is generated for transmission through the first pair of electrodes to the agonist muscle at a first intensity level for a period sufficient to initiate contraction of the agonist muscle, and then at a second intensity level which is less than the first intensity level for a period sufficient to continue contraction of the agonist muscle. A second pattern of electrical stimulation pulses is generated for transmission through the second pair of electrodes to the antagonist muscle at a first intensity level for a period sufficient to reduce the acceleration of the limb, and then at a second intensity level which is less than the first intensity level for a period sufficient to regulate the movement of the limb.

In order to facilitate an understanding of the invention, the preferred embodiments of the invention are illustrated in the drawings, and a detailed description thereof follows. It is not intended, however, that the invention be limited to the particular embodiments described or to use in connection with the apparatus illustrated herein. Various modifications and alternative embodiments such as would ordinarily occur to one skilled in the art to which the invention relates are also contemplated and included within the scope of the invention described and claimed herein.

BRIEF DESCRIPTION OF THE DRAWINGS

The presently preferred embodiments of the invention are illustrated in the accompanying drawings, in which like reference numerals represent like parts throughout, and in which:

5

FIG. 1 is a first embodiment of a device that may be used in applying neuromuscular electrical stimulation to an agonist/antagonist muscle pair to move a limb about a joint.

FIG. 2 is a front view of a portion of the device of FIG. 1, with the front access panel removed.

FIG. 3 is a rear view of the device of FIG. 1.

FIG. 4 is a bottom view of the device of FIG. 1.

FIG. 5 is an exploded perspective view of a second embodiment of an apparatus that may be used in applying neuromuscular electrical stimulation to an agonist/antagonist muscle pair to move a limb about a joint.

FIG. 6 is a front view of a module which comprises a portion of the apparatus of FIG. 5.

FIG. 7 is a bottom view of the module illustrated in FIGS. 5 and 6.

FIG. 8 is a block diagram illustrating the operation of the device of FIGS. 1-4 or the apparatus of FIGS. 5-7.

FIG. 9 is a perspective view of a patient's arm showing two pairs of electrodes which may be employed in the practice of a preferred embodiment of the invention.

FIG. 10 is a graphical illustration of patterns of electrical stimulation pulses which may be transmitted to an agonist muscle and corresponding patterns of electrical stimulation pulses which may be transmitted to the associated antagonist muscle according to a preferred embodiment of the invention. The X-axis shows elapsed time and the Y-axis shows the intensity of the electrical stimulation pulses.

FIG. 11 is a detailed illustration of one of the patterns of electrical stimulation pulses which may be transmitted to an agonist muscle and the corresponding pattern of electrical stimulation pulses which may be transmitted to the associated antagonist muscle according to a preferred embodiment of the invention. The X-axis shows elapsed time and the Y-axis shows the intensity of the electrical stimulation pulses.

DESCRIPTION OF THE PREFERRED EMBODIMENTS OF THE INVENTION

FIGS. 1-4 illustrate a preferred embodiment of a device for generating neuromuscular electrical stimulation for inducing muscle contraction in flexing or abducting a limb at a joint. As shown therein, device 20 comprises the main component of a modular system for providing the therapeutic application of energy in multiple forms. Device 20 comprises a combination two-channel electrotherapy and ultrasound system, which includes cabinet 22 having display screen 24. Device 20 also includes a user interface in the form of function keys 26 (including keys on both sides of the display screen), which form a part of the interactive interface of the device. Other function keys include knob 28 which provides therapy "Intensity Control" and button 30, which is a therapy session "Start" key. Button 32 is a therapy session "Pause" key and button 34 is a therapy session "Stop" key. Front access panel 36 provides access to a plurality of outlet jacks (shown in FIG. 2), including operator remote control connector 38, patient interrupt switch connector 40, electrical stimulation outlet jack 42 (comprised of channel 1 connector 44 and channel 2 connector 46), microcurrent probe connector 48 (for use when electrical stimulation is applied using a microcurrent waveform) and ultrasound applicator connector 50. The generators for the patterns of electrical stimulation pulses that are applied according to the invention are located in device 20.

FIG. 3 shows the rear of device 20 illustrating system power switch 52 and rear access panel 54, behind which is located the main power cord (not shown). FIG. 3 also shows the location of serial connector outlet jack 56 for connection of a serial device (not shown) such as a hand dynamometry

6

device, an electrogoniometry device or a pressure pad transducer. FIG. 4 shows the bottom of device 20, including a first module receiver which is adapted to receive several types of upgrade modules for enhancing the operation of the system.

This first module receiver comprises ribbon cable connector 58 to which an associated ribbon cable (not shown) may be attached. The first module receiver is adapted to receive an upgrade module such as a rechargeable battery module, a vacuum electrode module (which is adapted to permit the application of electrical stimulation using vacuum electrodes instead of adhesively applied electrodes), a module that is adapted to generate energy in the form of electromagnetic radiation (such as an LLLT module) or other types of upgrade modules. Referring again to FIG. 4, a second module receiver 60, which includes PC board contacts 62, is adapted to receive another type of upgrade module for enhancing the operation of device 20, such as an EMG module (not shown).

FIG. 5 illustrates an alternative embodiment of an apparatus for providing neuromuscular electrical stimulation according to the invention. As shown therein, device 120 is adapted to provide electrotherapy and/or ultrasound therapy, but does not provide the patterns of electrical stimulation pulses that are applied according to the invention without upgrade module 64. Device 120 includes cabinet 122 having display screen 124 and a user interface in the form of function keys 126 (including keys on both sides of the display screen), which form a part of the interactive interface of the device. Other function keys include knob 128 which provides therapy "Intensity Control" and button 130, which is a therapy session "Start" key. Button 132 is a therapy session "Pause" key and button 134 is a therapy session "Stop" key. Attached to device 120 is two-channel electrical stimulation upgrade module 64 for generating the electrical stimulation pulses that are applied through channels 1 and 2 according to the invention. Module 64 (also shown in FIGS. 6 and 7) includes ribbon cable connector 66 to which is attached one end of ribbon cable 68. The other end of ribbon cable 68 is attached to a first module receiver of device 120 (comprising a ribbon cable connector, not shown, but similar to ribbon cable connector 58 of device 20). Device 120 also includes front access panel 136 which is similar to, but larger than, front access panel 36 of device 20. As shown in FIG. 6, module 64 includes a plurality of outlet jacks, such as operator remote control connector 70, patient interrupt switch connector 72 and electrical stimulation outlet jack 74 (comprised of channel 1 connector 76 and channel 2 connector 78). FIG. 7 illustrates a bottom view of module 64. As shown therein, it is preferred that module 64 include secondary module receiver 80 which is essentially identical to second module receiver 60 of device 20. Secondary module receiver 80, which includes PC board contacts 82, is adapted to receive another type of upgrade module for enhancing the operation of the system, such as an EMG module.

Referring now to FIG. 8, the operation of the embodiment of FIGS. 1-4 or the embodiment of FIGS. 5-7 is illustrated. As shown therein, interface/main controller 90 is the control interface for the user and the primary controller for device 20 (or device 120 and attached module 64). Major components include a graphic display (such as display screen 24 of device 20 or display screen 124 of device 120), display controller, power supply controls, pushbuttons (including function keys 26 of device 20 or function keys 126 of device 120), and a power switch (such as power switch 52 of device 20). As described above, this interface allows the user to select the treatment parameters desired and to control the application of neuromuscular electrical stimulation during treatment.

Stimulation main controller **92** comprises the communication interface between stimulation channel **1** controller **104**, stimulation channel **2** controller **106** and user interface/main controller **90**. Stimulation controller **92** gets the treatment parameters from the user interface controller **90** and passes them on to the stimulator channels. Stimulation main controller **92** also passes operational parameters from stimulator channel **1** controller **104** and stimulation channel **2** controller **106** back to user interface/main controller **90**.

Ultrasound controller **98** provides the communication interface between ultrasound generator **100** and user interface/main controller **90**. Ultrasound controller **98** gets the treatment parameters from user interface controller **90** and sets up ultrasound generator **100** for proper output through ultrasound applicator **102**. The ultrasound controller also passes operational parameters from ultrasound generator **100** back to user interface/main controller **90**. Preferably, ultrasound generator **100** produces electrical energy at a frequency of approximately 1 MHz or 3.3 MHz. When connected to the ultrasound applicator it generates ultrasound at these frequencies. Stimulation from channel **2** output circuit can be routed through the ultrasound generator and out to the ultrasound applicator when so desired. This is accomplished with relay switch S1 and is engaged as shown in FIG. **8** (so that contact **2** is in electrical communication with contact **3**), when the user desires apply therapeutic treatment with both electrical stimulation and ultrasound simultaneously.

Stimulator channel **1** controller **104** controls stimulator channel **1** output circuitry **94** which generates the user selected waveform, including the electrical stimulation pulses that are applied through channel **1** according to the invention. Controller **104** controls and monitors both voltage and current passing to the patient through channel **1**, and it provides feedback status information to stimulator main controller **92**. Stimulator output circuit **94** for channel **1** is a variable high voltage power supply capable of generating voltages of up to 500 volts and continuous currents as high as 250 mA. The patient is connected to the output circuitry through switching devices that deliver stimulation based on the user selected waveform. The output can be controlled by maintaining either constant current or constant voltage. The output can also be dynamically controlled over time, varying in both amplitude and frequency.

Stimulator channel **2** controller **106** controls stimulator channel **2** output circuitry **96** which generates the user selected waveform, including the electrical stimulation pulses that are applied through channel **2** according to the invention. Controller **106** controls and monitors both voltage and current passing to the patient through channel **2**. Controller **106** also provides feedback status information to stimulator main controller **92**. Stimulator output circuit **96** for channel **2** is a variable high voltage power supply capable of generating voltages of up to 500 volts and continuous currents as high as 250 mA. The patient is connected to the output circuitry through switching devices that deliver stimulation based on the user selected waveform. Like the output from channel **1**, the output from channel **2** can be controlled by maintaining either constant current or constant voltage. The output can also be dynamically controlled over time, varying in both amplitude and frequency. The positive (+) output connection from channel **2** can be routed through ultrasound generator **100** to the ultrasound applicator when this mode of operation is selected by use of switch S1 so that contact **2** is in electrical communication with contact **1** (not shown).

The invention comprises a method and apparatus for applying neuromuscular electrical stimulation to an agonist/antagonist muscle pair to move a limb about a joint. Such

agonist/antagonist muscle pairs may include (among others) the biceps and triceps for moving the forearm about the elbow joint, finger flexors and finger extensors for moving the fingers about various finger joints, the wrist flexors and wrist extensors for moving the hand about the wrist joint, the quadriceps and hamstring for moving the lower leg about the knee joint and the anterior tibialis and gastroc/soleus for moving the foot about the ankle joint. According to the method of the invention, a device, such as device **20** or the device **120**/module **64** combination, is provided for generating a first pattern of neuromuscular electrical stimulation pulses for output through a first channel to a first pair of electrodes and a second pattern of neuromuscular stimulation pulses for output through a second channel to a second pair of electrodes. FIG. **9** illustrates the application of electrode **108** and electrode **109** from channel **1** to the skin over the wrist and finger flexor muscles (the agonist) of the forearm, although the relative positions of the electrodes of channel **1** may be reversed, or the electrodes may be placed in different positions. Electrode **108** is operatively attached to channel **1** output circuit **94** (shown in FIG. **8**) by electrode lead **110**, and electrode **109** is operatively attached to channel **1** output circuit **94** by electrode lead **111**. Similarly, electrode **112** and electrode **113** from channel **2** are applied to the skin over the wrist and finger extensor muscles (the antagonist) of the forearm, although the relative positions of the electrodes of channel **2** may be reversed, or the electrodes may be placed in different positions. Electrode **112** is operatively attached to channel **2** output circuit **96** (shown in FIG. **8**) by electrode lead **114**, and electrode **113** is operatively attached to channel **2** output circuit **96** by electrode lead **115**. The electrodes from each channel are preferably placed no further apart than the length (or diameter) of the smallest electrode. Preferably, the electrode pairs should be positioned longitudinally with respect to the direction of the muscle fibers. The electrodes of channel **1** are preferably placed on either end of the muscle bellies of the agonist muscle (or muscle group) and the electrodes of channel **2** are preferably placed on either end of the muscle bellies of the corresponding antagonist muscle (or muscle group).

When the first pair of electrodes **108** and **109** are properly attached to make electrical contact with the agonist muscles of the patient and to conduct neuromuscular electrical stimulation pulses from channel **1** output circuit **94** of device **20** (or the combination of device **120** and module **64**), and the second pair of electrodes **112** and **113** are properly attached to make electrical contact with the antagonist muscles of the patient and to conduct neuromuscular electrical stimulation pulses from channel **2** output circuit **96**, a first pattern **140** of electrical stimulation pulses (shown in FIGS. **10** and **11**) are generated for transmission through the first pair of electrodes to the agonist muscle, and a second pattern **142** of electrical stimulation pulses are generated for transmission through the second pair of electrodes to the antagonist muscle. Preferably, the first pattern of electrical stimulation comprises a series of pulses, each of which has a pulse duration within the range of 20-400 μ sec., most preferably within the range of 100-400 μ ec. It is also preferred that the second pattern of electrical stimulation comprises a series of pulses, each of which has a pulse duration within the range of 20-400 μ sec., and most preferably within the range of 100-400 μ sec. Further, it is preferred that the first pattern **140** of electrical stimulation pulses be generated during a plurality of first burst periods **148**, each of which has a duration within the range of 200-5000 msec., and that each first burst period be followed by a rest period or rest interval during which no electrical stimulation pulses are generated for transmission through the first

channel. Preferably, each first burst period **148** is followed by a rest period **150** which has a duration at least 2-5 times the duration of the preceding first burst period. Similarly, it is preferred that the second pattern **142** of electrical stimulation pulses be generated during a plurality of second burst periods **152**, each of which begins after the beginning of a first burst period and ends no later than (and most preferably simultaneously with) the end of the first burst period. It is also preferred that each of second burst periods **152** has a duration within the range of 200-5000 msec., and that each second burst period is followed by a rest period or rest interval during which no electrical stimulation pulses are generated for transmission through the second channel. Preferably, each second burst period **152** is followed by a rest period **154** which has a duration at least 2-5 times the duration of the preceding second burst period.

It is also preferred that the first pattern of electrical stimulation pulses be generated or provided in a waveform selected from the group consisting of symmetrical biphasic, asymmetrical biphasic, high volt and premodulated (most preferably symmetrical biphasic), and that the second pattern of electrical stimulation pulses be generated or provided in a waveform selected from the group consisting of symmetrical biphasic, asymmetrical biphasic, high volt and premodulated (most preferably symmetrical biphasic). Furthermore, it is preferred that first pulse pattern generating circuit **94** be adapted to generate a first pattern of electrical stimulation pulses having a frequency **144** within the range of 20-80 Hz and an intensity (or intensities) within the range of 10-150 mA., and that second pulse pattern generating circuit **96** be adapted to generate a second pattern of electrical stimulation pulses having a frequency **146** within the range of 20-80 Hz and an intensity (or intensities) within the range of 10-150 mA.

As shown in FIG. **11**, preferred first pulse pattern generating circuit **94** is adapted to generate a first pattern of electrical stimulation pulses for transmission through a first pair of electrodes **108** and **109** to the agonist muscle at a first intensity level **156** for a period **158** which is sufficient to initiate contraction of the agonist muscle, and at a second intensity level **160** which is less than the first intensity level (and most preferably 75-90% of the first intensity level) for a period **162** that is sufficient to continue contraction of the agonist muscle, and at a third intensity level which is greater than the second intensity level (and most preferably equal to the first intensity level **156**) for a period **164** that is sufficient to complete contraction of the agonist muscle. It is also contemplated within the scope of the invention that the first pattern of electrical stimulation pulses may be transmitted at a first intensity level **156** for a period **158** which is sufficient to initiate contraction of the agonist muscle, and at a somewhat lower intermediate intensity level **166** (preferably about 85% of the first intensity level) for a period **168**, and at a second intensity level **160** which is less than the first intensity level (preferably about 80% of the first intensity level) for a period **162** that is sufficient to continue contraction of the agonist muscle, and finally at a third intensity level which is greater than the second intensity level (and preferably equal to the first intensity level **156**) for a period **164** that is sufficient to complete contraction of the agonist muscle. Preferred first pulse pattern generating circuit **94** is also adapted to generate a first pattern of electrical stimulation pulses having period **162** of the second intensity level that is at least three times greater than period **158** of the first intensity level, and a period **164** of the third intensity level that is not greater than period **158** of the first intensity level.

Preferred second pulse pattern generating circuit **96** is adapted to generate a second pattern of electrical stimulation pulses for transmission through a second pair of electrodes **112** and **113** to the antagonist muscle, at a first intensity level **170** for a period **172** that is sufficient to reduce the acceleration of the limb, and at a second intensity level **174** which is less than the first intensity level (and most preferably 10-30% of the first intensity level) for a period **176** that is sufficient to regulate the movement of the limb, and at a third intensity level which is greater than the second intensity level (and preferably equal to first intensity level **170**) for a period **178** that is sufficient to stop the movement of the limb. Preferred second pulse pattern generating circuit **96** is also adapted to generate a second pattern of electrical stimulation pulses having a period **176** of the second intensity level that is 5-15 times greater than period **172** of the first intensity level and not more than five times greater than the period of the third intensity level, and having a period **178** of the third intensity level that is not more than three times greater than period **172** of the first intensity level.

Although this description contains many specifics, these should not be construed as limiting the scope of the invention but as merely providing illustrations of some of the presently preferred embodiments thereof, as well as the best mode contemplated by the inventor of carrying out the invention. The invention, as described herein, is susceptible to various modifications and adaptations, and the same are intended to be comprehended within the meaning and range of equivalents of the appended claims.

What is claimed is:

1. A device for applying neuromuscular electrical stimulation to an agonist/antagonist muscle pair to move a limb about a joint, said device comprising a main stimulator controller and a pulse pattern generating circuitry in communication with the main stimulator controller,

wherein the main stimulator controller is configured to control said pulse pattern generating circuitry to:

automatically generate, for each burst period of a plurality of burst periods, a first pattern of electrical stimulation pulses for transmission through a first pair of electrodes to the agonist muscle:

- (i) at a constant first current amplitude level for a period sufficient to initiate contraction of the agonist muscle,
- (ii) at a constant second current amplitude level, less than the first current amplitude level, for a period sufficient to continue contraction of the agonist muscle, the second current amplitude level period consecutive to the first current amplitude level period;

automatically generate, for each burst period of the plurality of burst periods, a second pattern of electrical stimulation pulses, different from the first pattern, for transmission through the second pair of electrodes to the antagonist muscle:

- (i) at a constant third current amplitude level for a period sufficient to reduce acceleration of the limb,
- (ii) at a constant fourth current amplitude level, less than the third current amplitude level, for a period sufficient to regulate movement of the limb, the fourth amplitude level period consecutive to the third current amplitude level period; and

wherein each burst period of the plurality of burst periods represents a predetermined period of time during which electrical stimulation is applied to the agonist/antagonist muscle pair.

11

2. The device of claim 1, wherein each burst period of the plurality of burst periods is followed by a predetermined rest period during which electrical stimulation is not applied to the agonist/antagonist muscle pair.

3. The device of claim 1, wherein each burst period of the plurality of burst periods further includes generating the first pattern of electrical stimulation pulses during a first burst period and generating the second pattern of electrical stimulation pulses during a second burst period that begins after a beginning of the first burst period and ends no later than an end of the first burst period.

4. The device of claim 1, wherein the second current amplitude level is 75-90% of the first current amplitude level, and wherein the fourth current amplitude level is 10-30% of the third current amplitude level.

5. The device of claim 1, wherein the period of the second current amplitude level is at least three times greater than the period of the first current amplitude level, and wherein the period of the fourth current amplitude level is 5-15 times greater than the period of the third current amplitude level.

6. The device of claim 1, wherein the first pattern of electrical stimulation pulses comprises a series of pulses, each of which has a pulse duration that is within a range of 20-400 μ sec, and wherein the second pattern of electrical stimulation pulses comprises a series of pulses, each of which has a pulse duration that is within a range of 20-400 μ sec.

7. The device of claim 1, wherein the first pattern of electrical stimulation pulses comprises a series of pulses generated at a frequency that is within a range of 20-80 Hz, and wherein the second pattern of electrical stimulation pulses comprises a series of pulses generated at a frequency that is within a range of 20-80 Hz.

8. The device of claim 1, wherein the electrical stimulation pulses in the first pattern of electrical stimulation pulses are generated at current amplitudes within a range of 10-150 mA, and wherein the electrical stimulation pulses in the second pattern of electrical stimulation pulses are generated at current amplitudes within a range of 10-150 mA.

9. The device of claim 1 wherein the first pattern of electrical stimulation pulses comprises a waveform selected from a group consisting of symmetrical biphasic, asymmetrical biphasic, high volt and premodulated, and wherein the second pattern of electrical stimulation pulses comprises a waveform selected from a group consisting of symmetrical biphasic, asymmetrical biphasic, high volt and premodulated.

10. The device of claim 1 wherein each burst period of the plurality of burst periods has a duration between 200 and 5000 msec.

11. The device of claim 1 wherein each burst period is followed by a predetermined rest period during which electrical stimulation is not applied to the agonist/antagonist muscle pair, and each rest period has a duration at least 2-5 times of a duration of the immediately preceding burst period.

12. A system for applying neuromuscular electrical stimulation to an agonist/antagonist muscle pair to move a limb about a joint,

wherein the system includes a main stimulator controller and a stimulation module comprising a pulse pattern generating circuitry in communication with the main stimulator controller,

wherein the stimulation module comprises patterns of electrical stimulation pulses, and wherein the main stimulator controller is configured to control said pulse pattern generating circuitry to:

automatically generate, for each burst period of a plurality of burst periods, a first pattern of electrical

12

stimulation pulses for transmission through a first pair of electrodes to the agonist muscle:

(i) at a constant first current amplitude level for a period sufficient to initiate contraction of the agonist muscle,

(ii) at a constant second current amplitude level, less than the first current amplitude level, for a period sufficient to continue contraction of the agonist muscle, the second current amplitude level period consecutive to the first current amplitude level period,

automatically generate, for each burst period of the plurality of burst periods, a second pattern of electrical stimulation pulses, different from the first pattern, for transmission through the second pair of electrodes to the antagonist muscle:

(i) at a constant third current amplitude level for a period sufficient to reduce acceleration of the limb,

(ii) at a constant fourth current amplitude level, less than the third current amplitude level, for a period sufficient to regulate movement of the limb, the fourth amplitude level period consecutive to the third current amplitude level period; and

wherein each burst period of the plurality of burst periods:

(i) represents a predetermined period of time during which electrical stimulation is applied to the agonist/antagonist muscle pair, and

(ii) is followed by a predetermined rest period during which electrical stimulation is not applied to the agonist/antagonist muscle pair.

13. The system of claim 12, wherein each burst period of the plurality of burst periods further includes generating the first pattern of electrical stimulation pulses during a first burst period and generating the second pattern of electrical stimulation pulses during a second burst period that begins after a beginning of the first burst period and ends no later than an end of the first burst period.

14. The system of claim 12, wherein each rest period has a duration at least 2-5 times of a duration of the immediately preceding burst period.

15. The device of claim 12, wherein the second current amplitude level is 75-90% of the first current amplitude level, and wherein the fourth current amplitude level is 10-30% of the third current amplitude level.

16. The device of claim 12, wherein the period of the second current amplitude level is at least three times greater than the period of the first current amplitude level, and wherein the period of the fourth current amplitude level is 5-15 times greater than the period of the third current amplitude level.

17. The device of claim 12, wherein the first pattern of electrical stimulation pulses comprises a series of pulses, each of which has a pulse duration that is within a range of 20-400 μ sec, and wherein the second pattern of electrical stimulation pulses comprises a series of pulses, each of which has a pulse duration that is within a range of 20-400 μ sec.

18. The device of claim 12, wherein the first pattern of electrical stimulation pulses comprises a series of pulses generated at a frequency that is within a range of 20-80 Hz, and wherein the second pattern of electrical stimulation pulses comprises a series of pulses generated at a frequency that is within a range of 20-80 Hz.

19. The device of claim 12, wherein the electrical stimulation pulses in the first pattern of electrical stimulation pulses are generated at current amplitudes within a range of 10-150 mA, and wherein the electrical stimulation pulses in the sec-

ond pattern of electrical stimulation pulses are generated at current amplitudes within a range of 10-150 mA.

20. The device of claim 12 wherein the first pattern of electrical stimulation pulses comprises a waveform selected from a group consisting of symmetrical biphasic, asymmetri- 5 cal biphasic, high volt and premodulated, and wherein the second pattern of electrical stimulation pulses comprises a waveform selected from a group consisting of symmetrical biphasic, asymmetrical biphasic, high volt and premodulated.

21. The device of claim 12 wherein each burst period of the 10 plurality of burst periods has a duration between 200 and 5000 msec.

* * * * *