

US009504467B2

(12) **United States Patent**  
**Ostrovsky et al.**

(10) **Patent No.:** **US 9,504,467 B2**  
(45) **Date of Patent:** **Nov. 29, 2016**

(54) **LESS TRAUMATIC METHOD OF DELIVERY OF MESH-BASED DEVICES INTO HUMAN BODY**

USPC ..... 606/193, 151, 139; 600/37; 604/273  
See application file for complete search history.

(75) Inventors: **Isaac Ostrovsky**, Wellesley, MA (US);  
**Jozef Slanda**, Milford, MA (US);  
**Jianmin Li**, Lexington, MA (US);  
**Brent Palmisano**, Fiskdale, MA (US);  
**James Goddard**, Pepperell, MA (US);  
**Daniel Ostrovsky**, Wellesley, MA (US)

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,843,272 A 2/1932 Evinrude  
2,204,265 A 6/1940 Wentzel  
2,466,282 A 4/1949 Sparrow et al.  
2,740,260 A 4/1956 Blanchard  
3,986,363 A 10/1976 Beaman et al.

(Continued)

FOREIGN PATENT DOCUMENTS

JP 2001260986 A 9/2001  
JP 2003098044 A 4/2003

(Continued)

OTHER PUBLICATIONS

Search Report and Written Opinion for International Patent Application No. PCT/US2010/061879, mailed on Mar. 21, 2011, 8 pages.

(Continued)

*Primary Examiner* — Richard Louis

(74) *Attorney, Agent, or Firm* — Brake Hughes Bellermann LLP

(73) Assignee: **Boston Scientific Scimed, Inc.**, Maple Grove, MN (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 518 days.

(21) Appl. No.: **12/978,140**

(22) Filed: **Dec. 23, 2010**

(65) **Prior Publication Data**

US 2011/0152914 A1 Jun. 23, 2011

**Related U.S. Application Data**

(60) Provisional application No. 61/289,898, filed on Dec. 23, 2009.

(51) **Int. Cl.**

**A61F 2/00** (2006.01)  
**A61B 17/06** (2006.01)  
**A61B 17/04** (2006.01)  
**A61B 17/00** (2006.01)

(52) **U.S. Cl.**

CPC ..... **A61B 17/06109** (2013.01); **A61B 17/0482** (2013.01); **A61B 2017/00805** (2013.01); **A61F 2/0045** (2013.01)



(58) **Field of Classification Search**

CPC ..... **A61B 17/06109**; **A61B 2017/00805**; **A61B 17/0482**; **A61F 2/2481**; **A61F 2/0045**

(57) **ABSTRACT**

In some embodiments, a method includes extending a dilator into a body of a patient in a first direction such that a distal end portion of the dilator extends from the body. The dilator defines a lumen therethrough. At least a portion of the dilator is disposed within the body when the distal end portion extends from the body. At least a portion of an implant is passed through the lumen defined by the dilator. The dilator is removed from the body by moving the dilator in the first direction.

**16 Claims, 15 Drawing Sheets**

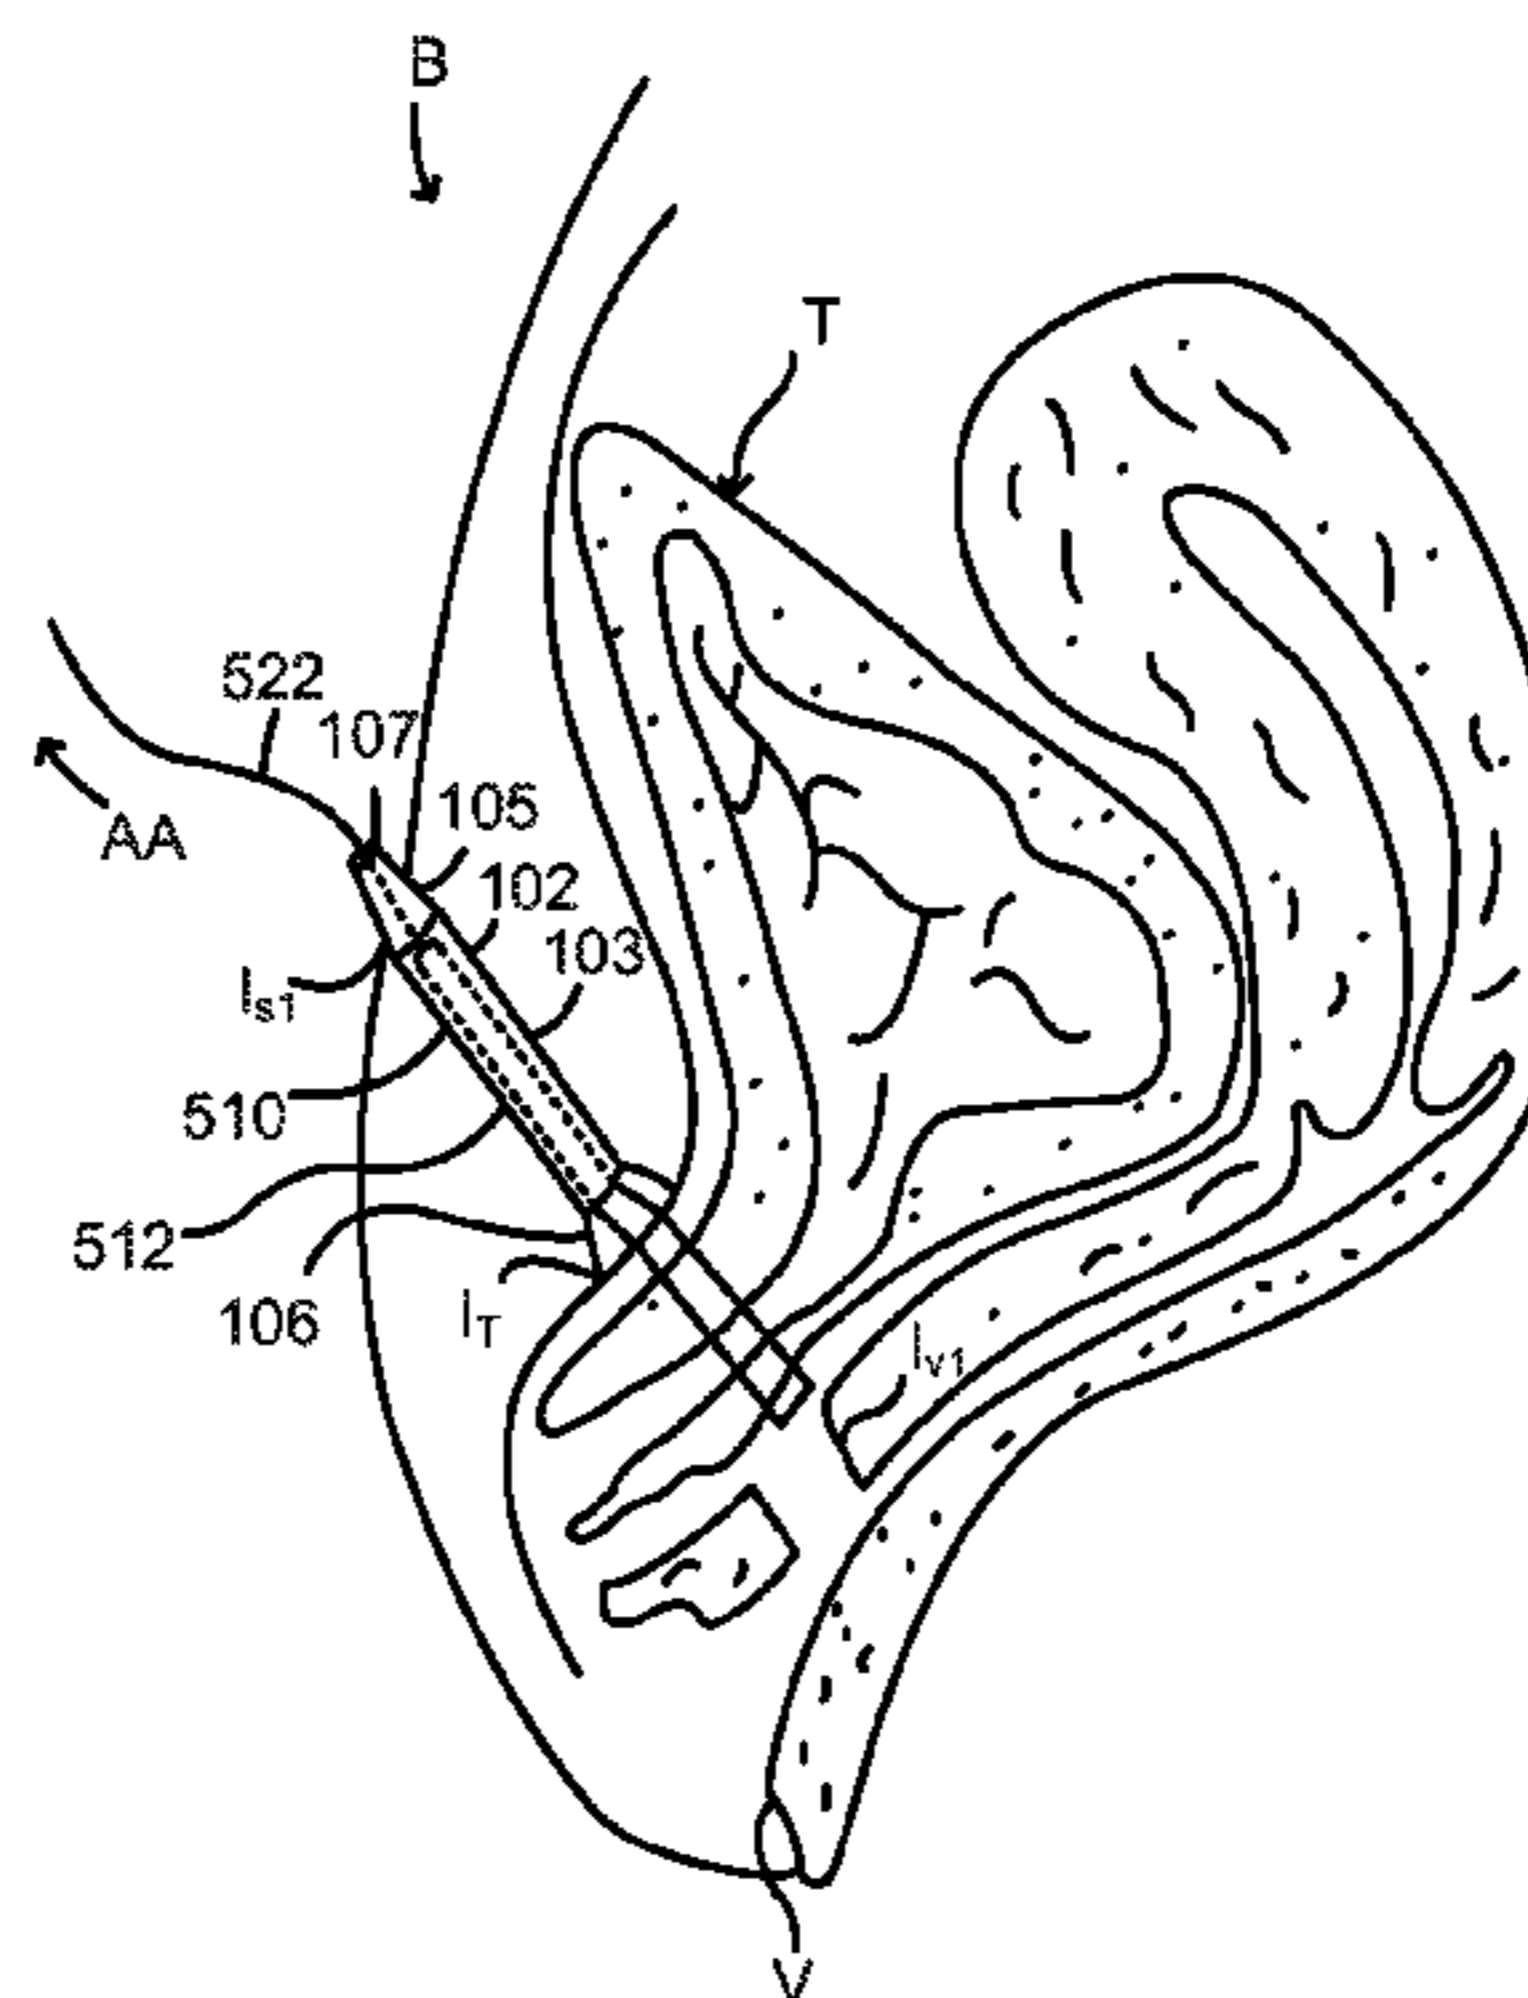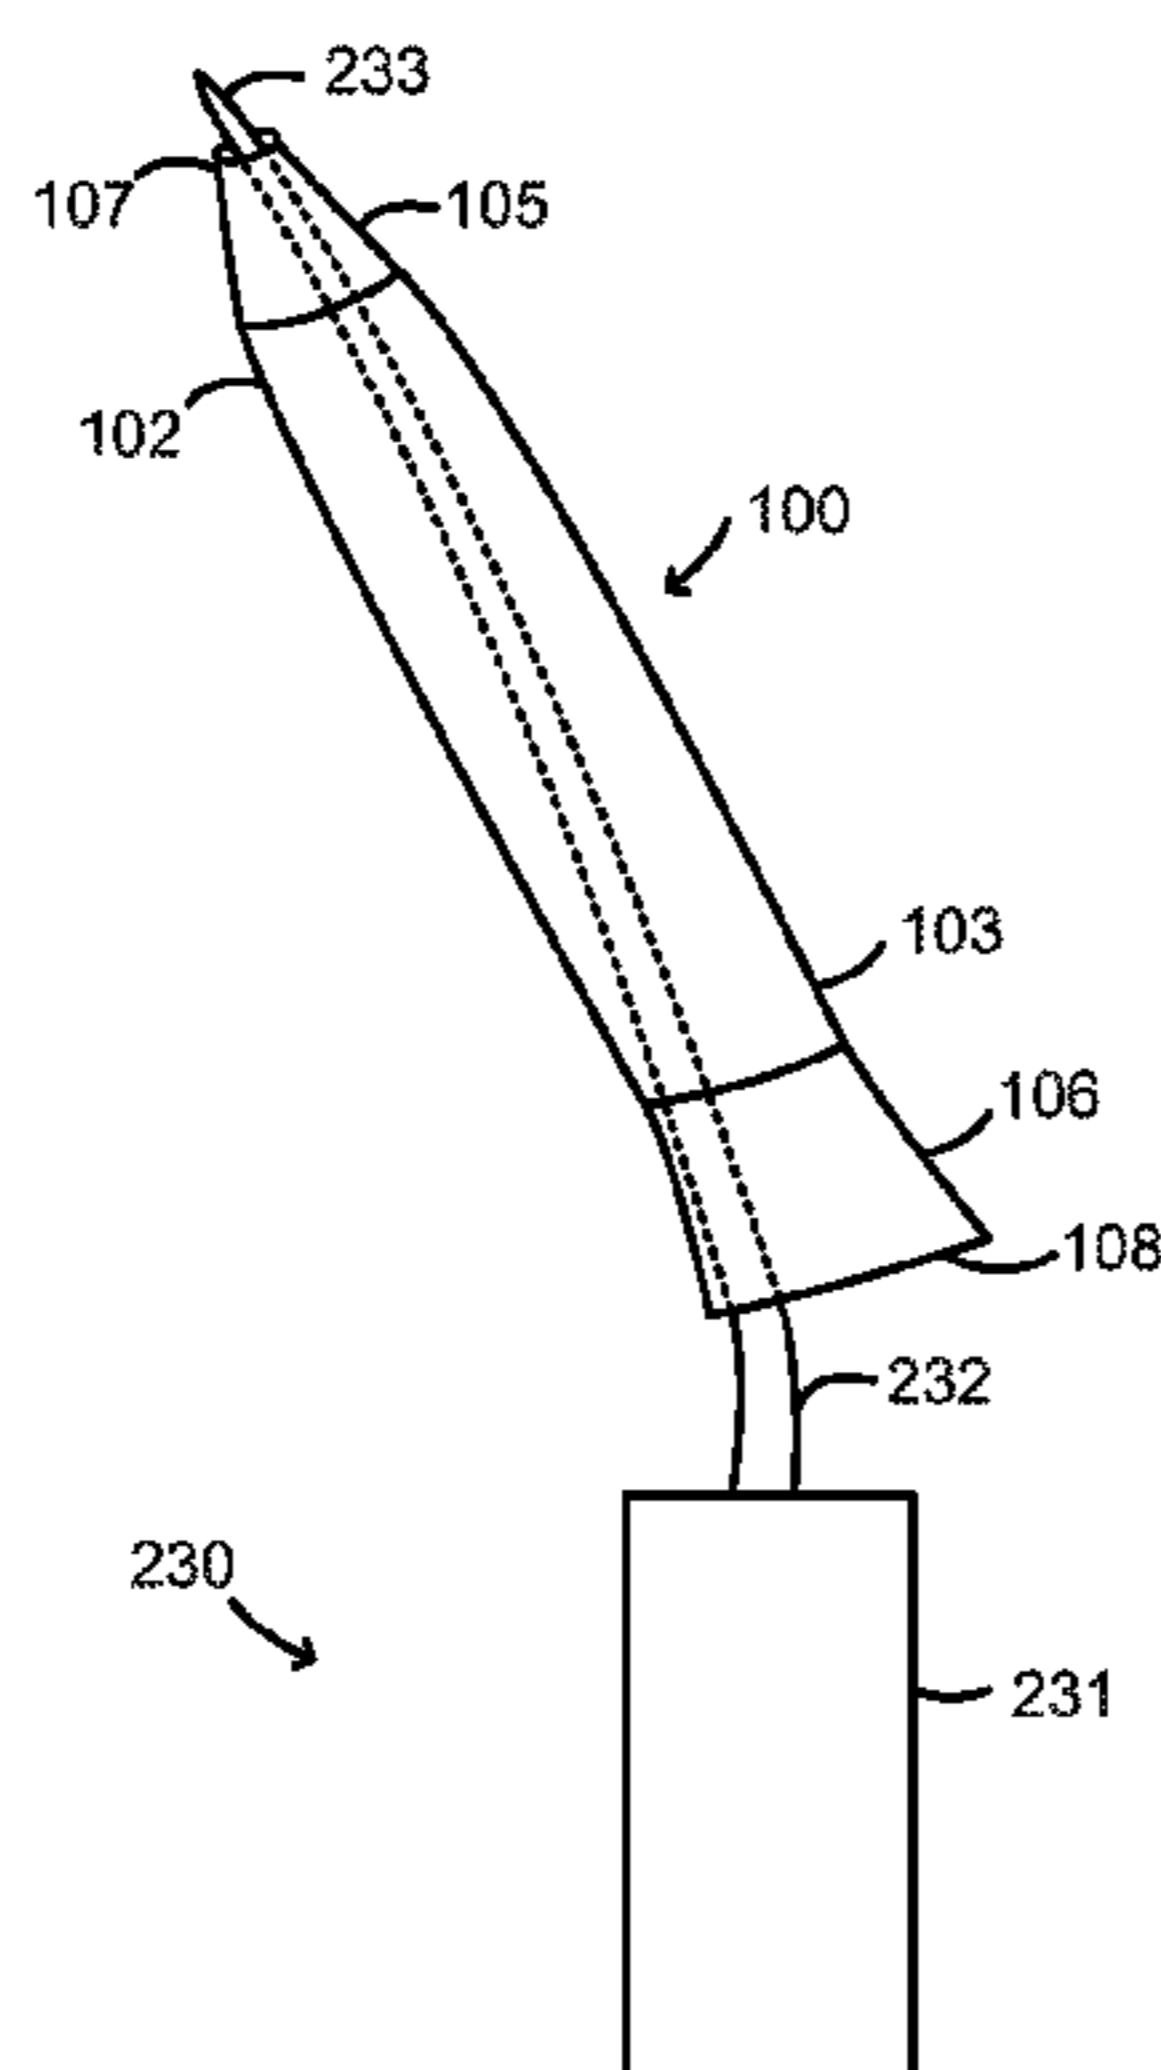

(56)

## References Cited

## U.S. PATENT DOCUMENTS

4,412,422 A	11/1983	Rossi	6,132,438 A	10/2000	Fleishman et al.
4,622,938 A	11/1986	Wenstadt et al.	6,233,943 B1	5/2001	Beacom et al.
4,646,696 A	3/1987	Dogadko	6,273,771 B1	8/2001	Buckley et al.
4,648,497 A	3/1987	Prince	6,280,269 B1	8/2001	Gaynor
4,747,381 A	5/1988	Baltz et al.	6,322,804 B1	11/2001	Dionne et al.
4,755,156 A	7/1988	Wagner	6,351,704 B1	2/2002	Koerner
4,788,955 A	12/1988	Wood	6,361,559 B1	3/2002	Houser et al.
4,801,282 A	1/1989	Ogawa et al.	6,379,114 B1	4/2002	Schott et al.
4,805,396 A	2/1989	Veerhusen et al.	6,379,366 B1	4/2002	Fleischman et al.
4,809,506 A	3/1989	Lauritsen	6,382,122 B1	5/2002	Gaynor et al.
4,810,216 A	3/1989	Kawamura	6,385,586 B1	5/2002	Dietz
4,836,809 A	6/1989	Pelligrino	6,414,607 B1	7/2002	Gonring et al.
4,850,906 A	7/1989	Kanno	6,423,080 B1	7/2002	Gellman et al.
4,858,585 A	8/1989	Remmers	6,587,765 B1	7/2003	Graham et al.
4,898,045 A	2/1990	Baba	6,599,302 B2	7/2003	Houser et al.
4,964,276 A	10/1990	Sturdy	6,612,882 B2	9/2003	Shidara et al.
5,004,962 A	4/1991	Fonss et al.	6,689,047 B2	2/2004	Gellman
5,051,102 A	9/1991	Onoue	6,689,062 B1	2/2004	Mesallum
5,062,403 A	11/1991	Breckenfeld et al.	6,704,643 B1	3/2004	Suhre et al.
5,062,516 A	11/1991	Prince et al.	6,719,781 B1	4/2004	Kim
5,065,723 A	11/1991	Broughton et al.	6,734,285 B2	5/2004	Hu et al.
5,103,946 A	4/1992	Masters et al.	6,740,101 B2	5/2004	Houser et al.
5,112,344 A	5/1992	Petros	6,751,533 B2	6/2004	Graham et al.
5,157,956 A	10/1992	Isaji et al.	6,752,814 B2	6/2004	Gellman et al.
5,167,212 A	12/1992	Peter et al.	6,830,052 B2	12/2004	Carter et al.
5,273,016 A	12/1993	Gillespie et al.	6,830,576 B2	12/2004	Fleishman et al.
5,318,466 A	6/1994	Nagafusa	6,843,795 B1	1/2005	Houser et al.
5,381,769 A	1/1995	Nishigaki et al.	6,887,249 B1	5/2005	Houser et al.
5,492,493 A	2/1996	Ohkita	6,910,927 B2	6/2005	Kanno
5,496,332 A	3/1996	Sierra et al.	6,960,351 B2	11/2005	Dionne et al.
5,539,294 A	7/1996	Kobayashi	6,965,817 B2	11/2005	Graham et al.
5,595,159 A	1/1997	Huber et al.	7,014,607 B2	3/2006	Gellman
5,611,515 A	3/1997	Benderev et al.	7,101,366 B2	9/2006	Trout, III et al.
5,664,542 A	9/1997	Kanazava et al.	7,121,908 B2	10/2006	Okuyama
5,676,670 A	10/1997	Kim	7,142,955 B1	11/2006	Kern et al.
5,730,105 A	3/1998	McGinnity	7,153,174 B2	12/2006	Takada et al.
5,733,325 A	3/1998	Robinson et al.	7,153,942 B2	12/2006	Hu et al.
5,749,343 A	5/1998	Nichols et al.	7,156,863 B2	1/2007	Sonnenschein et al.
5,771,860 A	6/1998	Bernardi	7,182,771 B1	2/2007	Houser et al.
5,774,854 A	6/1998	Sharman	7,186,688 B1	3/2007	Hu et al.
5,782,659 A	7/1998	Motose	7,208,582 B2	4/2007	Rosen et al.
5,797,920 A	8/1998	Kim	7,220,153 B2	5/2007	Okuyama
5,798,113 A	8/1998	Dionne et al.	7,235,094 B2	6/2007	Serino et al.
5,800,828 A	9/1998	Dionne et al.	7,273,751 B2	9/2007	Coleman
5,800,829 A	9/1998	Dionne et al.	7,297,144 B2	11/2007	Fleishman et al.
5,834,001 A	11/1998	Dionne et al.	7,303,525 B2	12/2007	Watschke et al.
5,837,234 A	11/1998	Gentil et al.	7,377,938 B2	5/2008	Sarac et al.
5,842,478 A	12/1998	Benderev et al.	7,393,320 B2	7/2008	Montpetit et al.
5,860,425 A	1/1999	Benderev et al.	7,402,312 B2	7/2008	Rosen et al.
5,865,791 A	2/1999	Whayne et al.	7,413,540 B2	8/2008	Gellman et al.
5,869,077 A	2/1999	Dionne et al.	7,439,333 B2	10/2008	Hu et al.
5,871,767 A	2/1999	Dionne et al.	7,485,092 B1	2/2009	Stewart et al.
5,874,099 A	2/1999	Dionne et al.	7,524,281 B2	4/2009	Chu et al.
5,891,193 A	4/1999	Robinson et al.	7,572,257 B2	8/2009	Whayne et al.
5,899,191 A	5/1999	Rabbit et al.	7,578,839 B2	8/2009	Serino et al.
5,899,909 A	5/1999	Claren et al.	2001/0018549 A1	8/2001	Scetbon
5,935,161 A	8/1999	Robinson et al.	2001/0056282 A1	12/2001	Sonnenschein et al.
5,984,917 A	11/1999	Fleischman et al.	2002/0193448 A1	12/2001	Wallace et al.
6,004,347 A	12/1999	McNamara et al.	2002/0032462 A1	3/2002	Houser et al.
6,007,544 A	12/1999	Kim	2002/0055748 A1	5/2002	Gellman et al.
6,015,319 A	1/2000	Tanaka	2002/0058959 A1*	5/2002	Gellman ..... A61B 17/0401 606/185
6,026,783 A	2/2000	Nestvall et al.	2002/0082627 A1	6/2002	Berg et al.
6,039,686 A	3/2000	Kovac	2002/0090388 A1	7/2002	Humes et al.
6,040,157 A	3/2000	Hu et al.	2002/0090389 A1	7/2002	Humes et al.
6,042,534 A	3/2000	Gellman et al.	2002/0099258 A1*	7/2002	Staskin ..... A61B 17/3468 600/29
6,058,349 A	5/2000	Kikori et al.	2002/0099394 A1	7/2002	Houser et al.
6,066,325 A	5/2000	Wallace et al.	2002/0111636 A1	8/2002	Fleischman et al.
6,073,509 A	6/2000	Salecker et al.	2002/0150603 A1	10/2002	Dionne et al.
6,073,592 A	6/2000	Brown et al.	2002/0156487 A1	10/2002	Gellman et al.
6,077,297 A	6/2000	Robinson et al.	2002/0156488 A1	10/2002	Gellman et al.
6,083,523 A	7/2000	Dionne et al.	2002/0173808 A1	11/2002	Houser et al.
6,095,488 A	8/2000	Semeyn, Jr. et al.	2002/0173809 A1	11/2002	Fleishman et al.
6,098,591 A	8/2000	Iwata	2003/0008357 A1	1/2003	Hu et al.
6,109,986 A	8/2000	Gaynor et al.	2003/0028007 A1	2/2003	Hu et al.
6,110,101 A	8/2000	Tihon et al.	2003/0033005 A1	2/2003	Houser et al.
			2003/0062052 A1	4/2003	Carter et al.
			2003/0082962 A1	5/2003	Kanno

(56)

References Cited

U.S. PATENT DOCUMENTS

2003/0092331 A1 5/2003 Okuyama  
 2003/0093196 A1 5/2003 Okuyama  
 2003/0167064 A1 9/2003 Whayne  
 2003/0170786 A1 9/2003 Rosen et al.  
 2003/0175274 A1 9/2003 Rosen et al.  
 2003/0176674 A1 9/2003 Rosen et al.  
 2003/0176875 A1\* 9/2003 Anderson et al. .... 606/151  
 2003/0195607 A1 10/2003 Trout et al.  
 2003/0212305 A1\* 11/2003 Anderson et al. .... 600/29  
 2003/0215921 A1 11/2003 Coleman  
 2004/0002679 A1 1/2004 Trout et al.  
 2004/0029461 A1 2/2004 Shomura  
 2004/0039246 A1 2/2004 Gellman et al.  
 2004/0064014 A1 4/2004 Melvin et al.  
 2004/0078053 A1 4/2004 Berg et al.  
 2004/0097801 A1 5/2004 Mesallum  
 2004/0097993 A1 5/2004 Whayne  
 2004/0106845 A1\* 6/2004 Anderson et al. .... 600/30  
 2004/0106846 A1\* 6/2004 Gellman ..... 600/30  
 2004/0111145 A1 6/2004 Serino et al.  
 2004/0116944 A1 6/2004 Chu et al.  
 2004/0143103 A1 7/2004 Hu et al.  
 2004/0185083 A1 9/2004 Dionne et al.  
 2004/0199177 A1 10/2004 Kim  
 2004/0225181 A1\* 11/2004 Chu et al. .... 600/37  
 2004/0230206 A1 11/2004 Gellman et al.  
 2004/0230207 A1 11/2004 Gellman et al.  
 2004/0236314 A1 11/2004 Saab  
 2004/0236411 A1 11/2004 Sarac et al.  
 2005/0033321 A1 2/2005 Fleischman et al.  
 2005/0043580 A1 2/2005 Watschke et al.  
 2005/0059117 A1 3/2005 Rosen et al.  
 2005/0090706 A1 4/2005 Gellman et al.  
 2005/0110214 A1 5/2005 Shank et al.  
 2005/0113904 A1 5/2005 Shank et al.  
 2005/0118895 A1 6/2005 Kanno et al.  
 2005/0148818 A1 7/2005 Mesallum  
 2005/0176103 A1 8/2005 Hu et al.  
 2005/0192429 A1 9/2005 Rosen et al.  
 2005/0197525 A1 9/2005 Gellman  
 2005/0232921 A1 10/2005 Rosen et al.  
 2005/0245145 A1 11/2005 Takada et al.  
 2005/0245787 A1\* 11/2005 Cox et al. .... 600/37  
 2005/0251244 A1 11/2005 Vounderwalde  
 2005/0267325 A1 12/2005 Bouchier et al.  
 2005/0286539 A1 12/2005 Okuyama  
 2006/0025331 A1 2/2006 Hu et al.  
 2006/0025649 A1\* 2/2006 Smith et al. .... 600/30  
 2006/0041185 A1\* 2/2006 Browning ..... 600/37  
 2006/0057117 A1 3/2006 Coleman  
 2006/0074484 A1 4/2006 Huber  
 2006/0122620 A1 6/2006 Kim  
 2006/0161110 A1 7/2006 Lenker et al.  
 2006/0177478 A1 8/2006 Humes et al.  
 2006/0195011 A1 8/2006 Arnal et al.  
 2006/0229493 A1\* 10/2006 Weiser ..... A61B 17/00234  
 600/37  
 2006/0240720 A1 10/2006 Yamashita et al.  
 2006/0253132 A1 11/2006 Evans et al.  
 2006/0253152 A1 11/2006 Evans et al.  
 2006/0258898 A1 11/2006 Montpetit et al.  
 2006/0260618 A1\* 11/2006 Hodroff ..... A61B 17/06066  
 128/830  
 2006/0287673 A1 12/2006 Brett et al.  
 2006/0293646 A1 12/2006 Whayne et al.  
 2007/0010807 A1 1/2007 Chu  
 2007/0010830 A1 1/2007 Gellman et al.  
 2007/0010875 A1 1/2007 Trout et al.  
 2007/0021649 A1 1/2007 Nowlin et al.  
 2007/0021760 A1 1/2007 Kelleher  
 2007/0043374 A1 2/2007 Evans  
 2007/0060788 A1 3/2007 Gellman  
 2007/0082565 A1 4/2007 Okuyama  
 2007/0092489 A1 4/2007 Fishbein et al.  
 2007/0129751 A1 6/2007 Muni et al.

2007/0149999 A1 6/2007 Szabo et al.  
 2007/0173926 A1 7/2007 Bobo et al.  
 2007/0178780 A1 8/2007 Ito et al.  
 2007/0203517 A1 8/2007 Williams et al.  
 2007/0218785 A1 9/2007 Okuyama et al.  
 2007/0219620 A1 9/2007 Eells et al.  
 2007/0225642 A1 9/2007 Houser et al.  
 2007/0227429 A1 10/2007 Okuyama et al.  
 2007/0232162 A1 10/2007 Okuyama et al.  
 2007/0249244 A1 10/2007 Watanabe et al.  
 2007/0250222 A1 10/2007 Okuyama et al.  
 2007/0270055 A1 11/2007 Ito et al.  
 2007/0282490 A1 12/2007 Ito et al.  
 2007/0293102 A1 12/2007 Okuyama et al.  
 2008/0003898 A1 1/2008 Watanabe et al.  
 2008/0009747 A1 1/2008 Saadat et al.  
 2008/0015569 A1 1/2008 Saadat et al.  
 2008/0033457 A1 2/2008 Francischelli et al.  
 2008/0046005 A1 2/2008 Lenker et al.  
 2008/0066769 A1 3/2008 Dineen et al.  
 2008/0077174 A1 3/2008 Mische  
 2008/0097487 A1 4/2008 Pool et al.  
 2008/0097488 A1 4/2008 Fleischman et al.  
 2008/0097496 A1 4/2008 Chang et al.  
 2008/0125621 A1\* 5/2008 Gellman et al. .... 600/37  
 2008/0125791 A1 5/2008 Gellman et al.  
 2008/0146867 A1 6/2008 Gellman et al.  
 2008/0187604 A1 8/2008 Tomaselli et al.  
 2008/0199541 A1 8/2008 Tomaselli et al.  
 2008/0221386 A1 9/2008 Gellman et al.  
 2008/0269552 A1 10/2008 Montpetit et al.  
 2008/0286250 A1 11/2008 Tornoe et al.  
 2008/0286288 A1 11/2008 Rosen et al.  
 2008/0286323 A1 11/2008 Tornoe et al.  
 2008/0287740 A1 11/2008 Weitzner et al.  
 2009/0018387 A1 1/2009 Veronikis  
 2009/0023224 A1 1/2009 Rosenig et al.  
 2009/0023986 A1 1/2009 Stewart et al.  
 2009/0024072 A1 1/2009 Criado et al.  
 2009/0043356 A1 2/2009 Longhini et al.  
 2009/0054970 A1 2/2009 Houser et al.  
 2009/0093672 A1\* 4/2009 Chu ..... A61B 17/06109  
 600/37  
 2009/0104248 A1 4/2009 Rapacki et al.  
 2009/0132025 A1 5/2009 Shank et al.  
 2009/0137861 A1 5/2009 Goldberg et al.  
 2009/0143789 A1 6/2009 Houser  
 2009/0143808 A1 6/2009 Houser  
 2009/0156891 A1 6/2009 Heys et al.  
 2009/0171139 A1 7/2009 Chu  
 2009/0171140 A1\* 7/2009 Chu ..... A61B 17/0482  
 600/37  
 2009/0192347 A1\* 7/2009 Davila et al. .... 600/37  
 2009/0198172 A1 8/2009 Garrison et al.  
 2010/0198003 A1\* 8/2010 Morningstar et al. .... 600/37

FOREIGN PATENT DOCUMENTS

JP 2003127986 A 5/2003  
 JP 2003146293 A1 5/2003  
 JP 2004068704 A 3/2004  
 JP 2004244003 A 9/2004  
 JP 2005297785 A 10/2005  
 WO 2004/016180 A2 2/2004  
 WO 2005/102833 A1 11/2005  
 WO 2011/079222 A2 6/2011

OTHER PUBLICATIONS

“Suprapubic Mid-Urethral Sling System”, Lynx, Boston Scientific ,  
 Apr. 29, 2004, 4 pages.  
 “Solyx SIS Systems: The Carrier Tip that Allows for Advanced  
 Control”, Boston Scientific, Copyright 2009, retrieved on Oct. 22,  
 2009 from <http://www.bostonscientific.com>, 2 pages.  
 “Solyx SIS Systems: Advanced Control with Micro Adjustability”,  
 Boston Scientific, Copyright 2009, 4 pages.

(56)

**References Cited**

OTHER PUBLICATIONS

“Advantage: Transvaginal Mid-Urethral Sling System”, Boston Scientific, Copyright 2003, 4 pages.

Kohli, “A Minimally Invasive Approach to Anterior Wall Reconstruction for Incontinence and Prolapse: Four Corner Cystocele Repair With Repliform Graft Combined with Advantage Mid-Urethral Sling”, Boston Scientific, Copyright 2004, 4 pages.

“Advantage: Transvaginal Mid-Urethral Sling System”, Boston Scientific, Copyright 2009, retrieved on Oct. 22, 2009 from <http://www.bostonscientific.com>, 2 pages.

Kleeman, Steve, “Obtryx: Transobturator System Featuring Advantage Mesh”, Boston Scientific, Copyright 2006, 4 pages.

“Obtryx: Transobturator Mid-Urethral Sling System”, Boston Scientific, Copyright 2009, retrieved on Oct. 22, 2009 from <http://www.bostonscientific.com>, 2 pages.

“Obtryx: Transobturator Mid-Urethral Sling System”, Boston Scientific, Copyright 2008, 4 pages.

Leach, “Obtryx Sling System”, Boston Scientific, Copyright 2006, 4 pages.

Nilsson, C. G., et al., “The Tension-free Vaginal Tape Procedure is Successful in the Majority of Women with Indications for Surgical Treatment of Urinary Stress Incontinence”, *British Journal of Obstetrics and Gynecology*, vol. 108, Apr. 2001, pp. 414-419.

Atherton, M. J., et al., “A Comparison of Bladder Neck Movement and Elevation After Tension-free Vaginal Tape and Colposuspension”, *British Journal of Obstetrics and Gynecology*, vol. 107, Nov. 2000, pp. 1366-1370.

Ulmsten, et al., “An Ambulatory Surgical Procedure Under Local Anesthesia for Treatment of Female Urinary Incontinence”, *International Urogynecology Journal*, vol. 7, No. 2, 1996, pp. 81-86.

\* cited by examiner

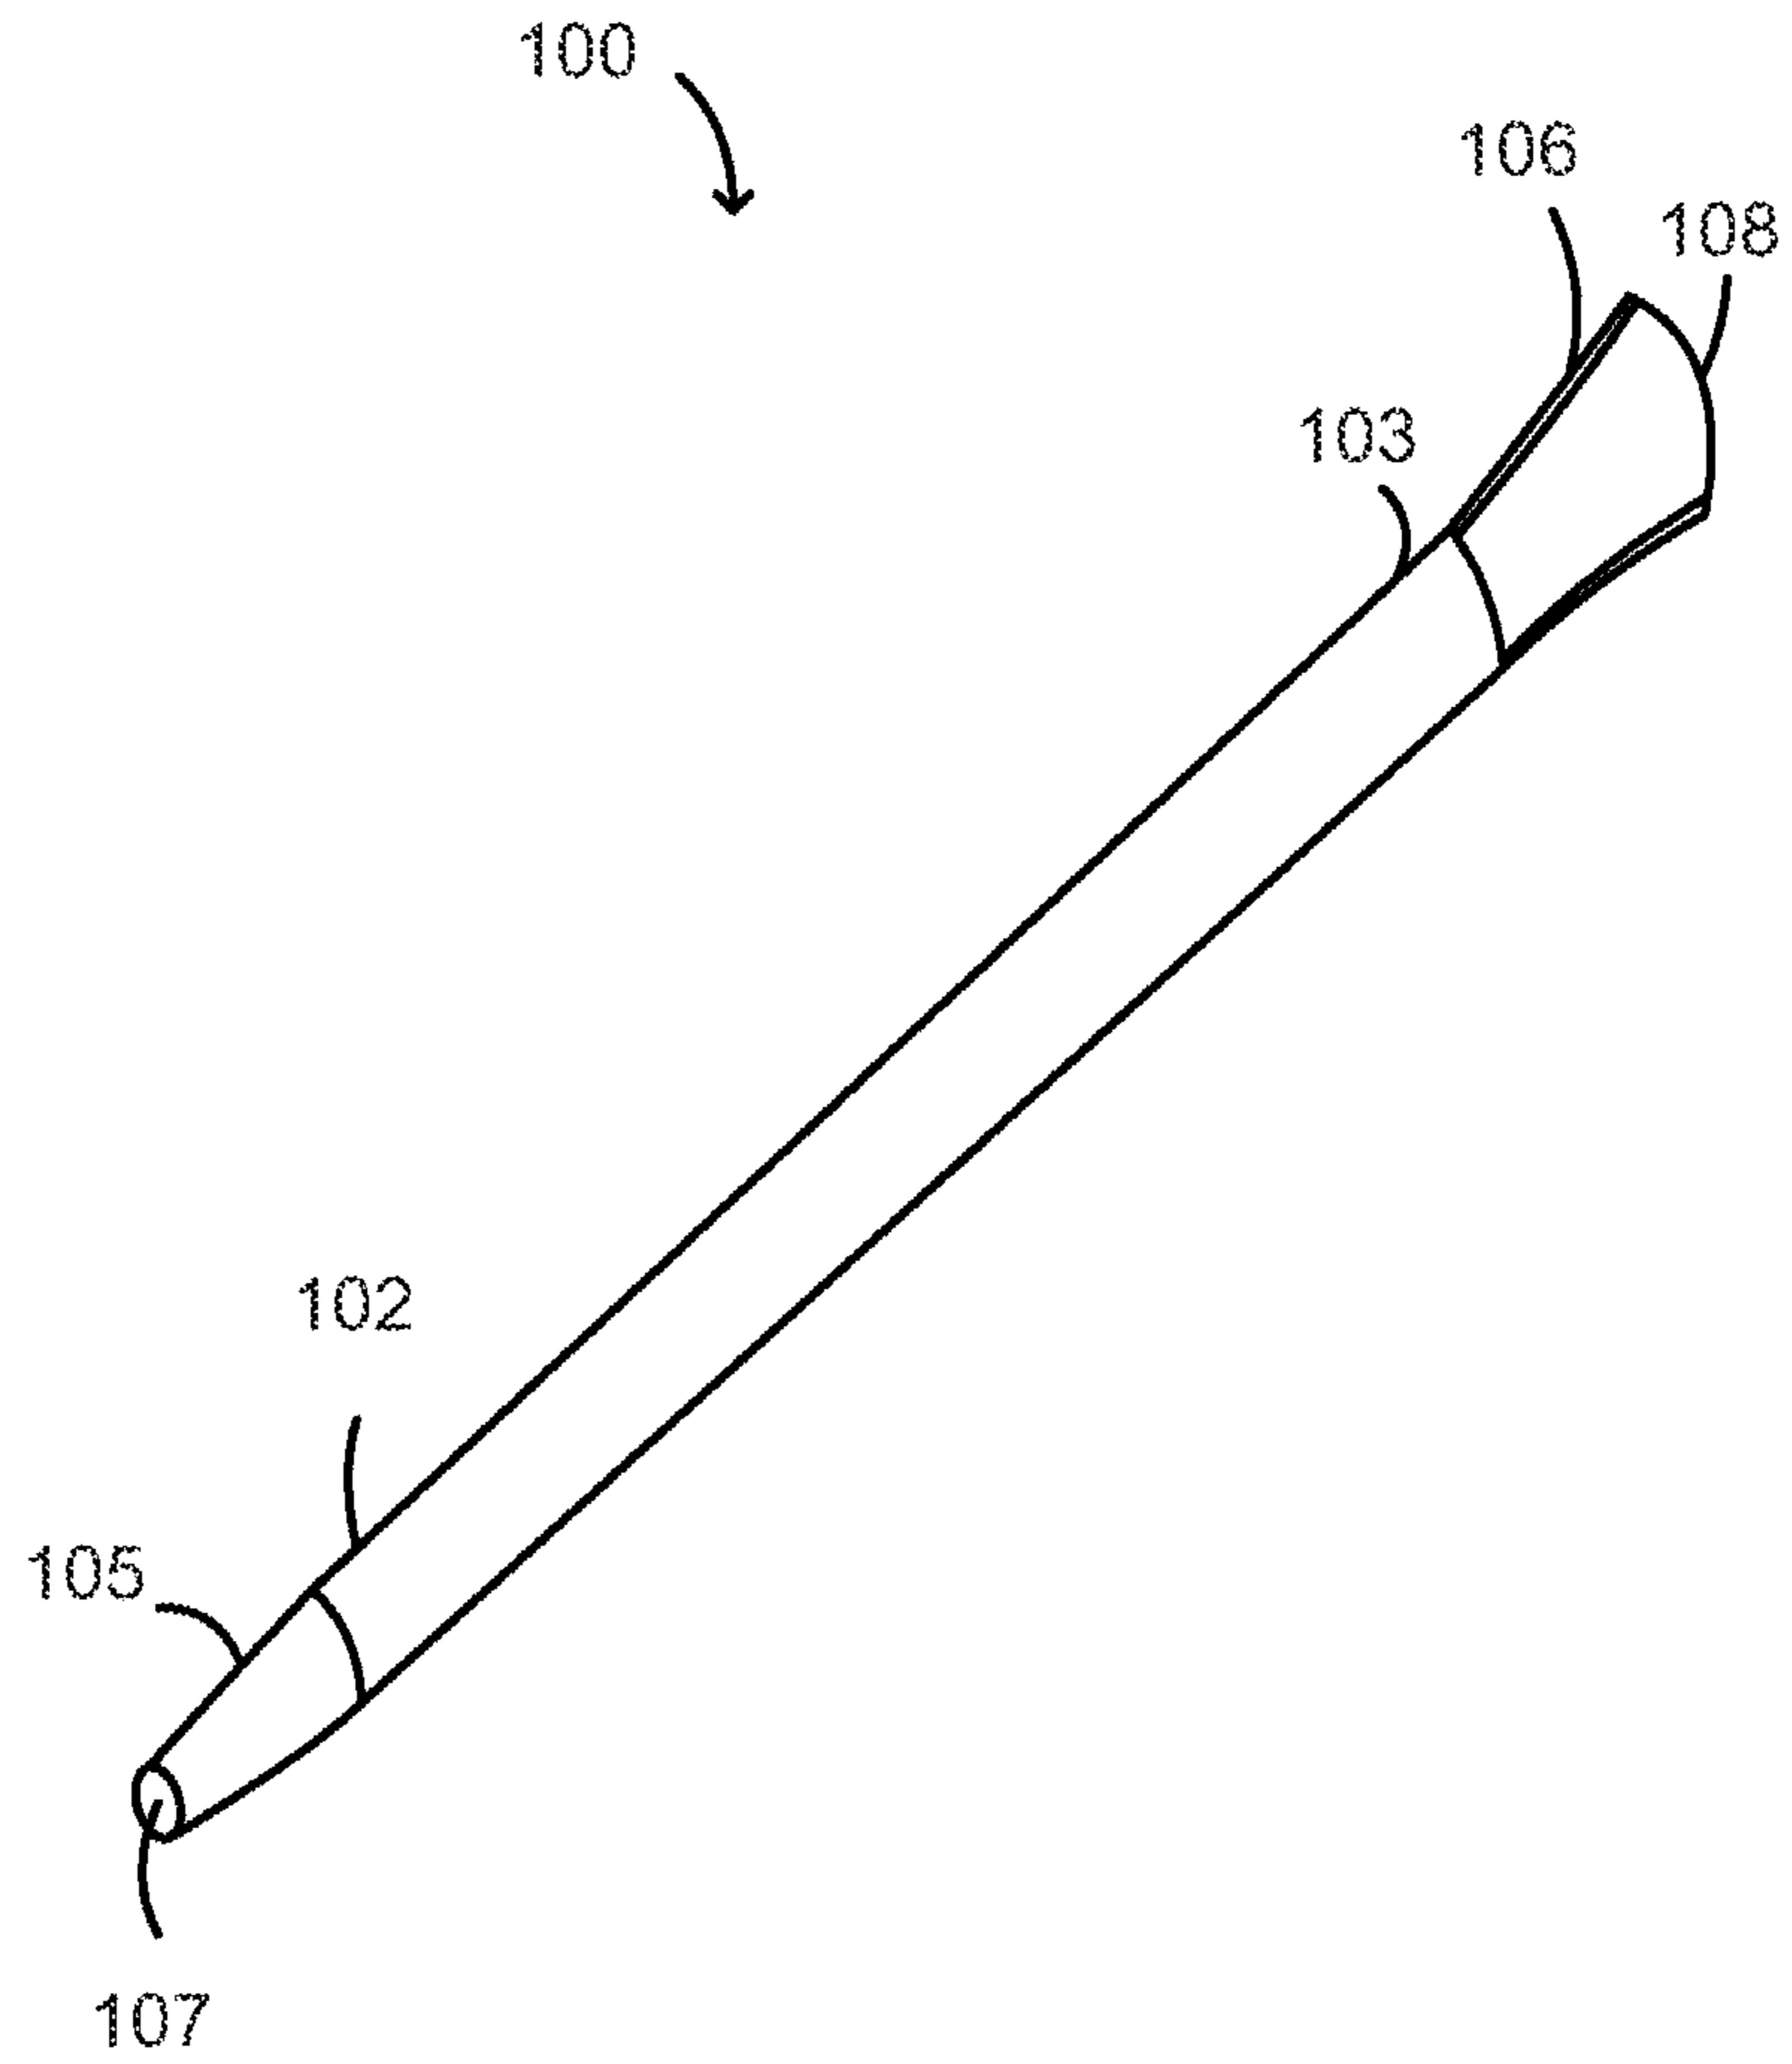


FIG. 1

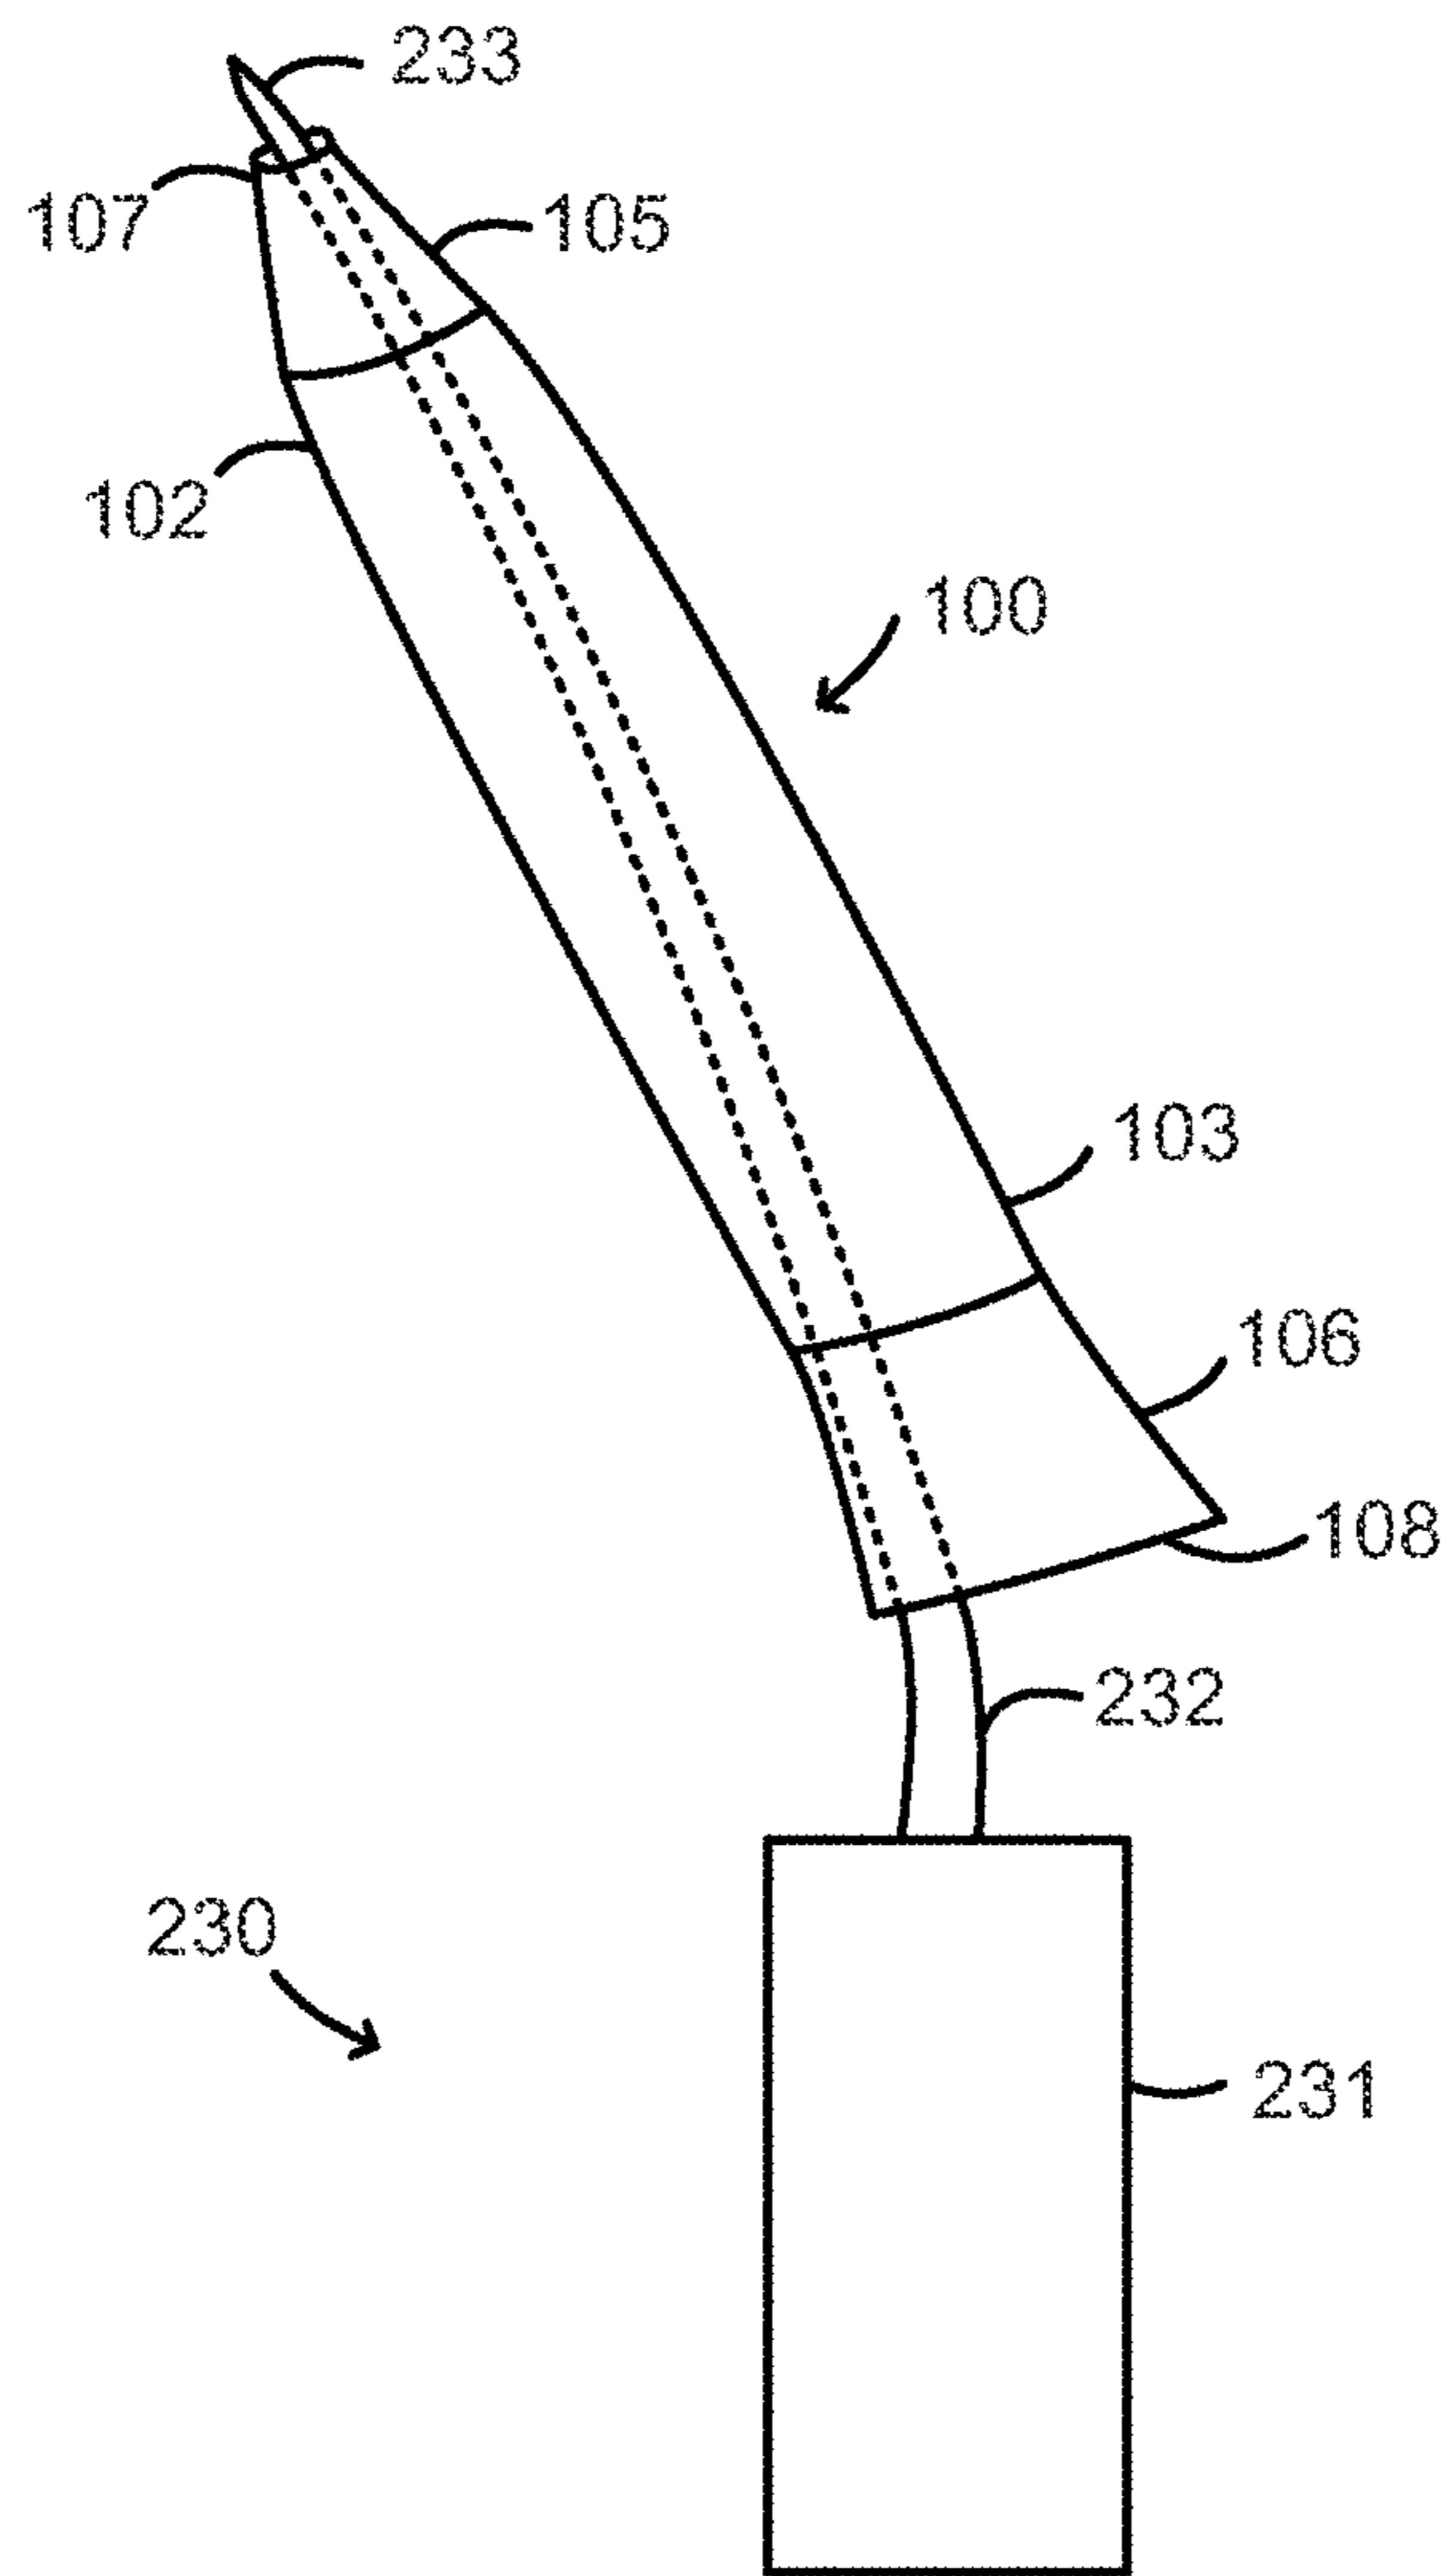


FIG. 2

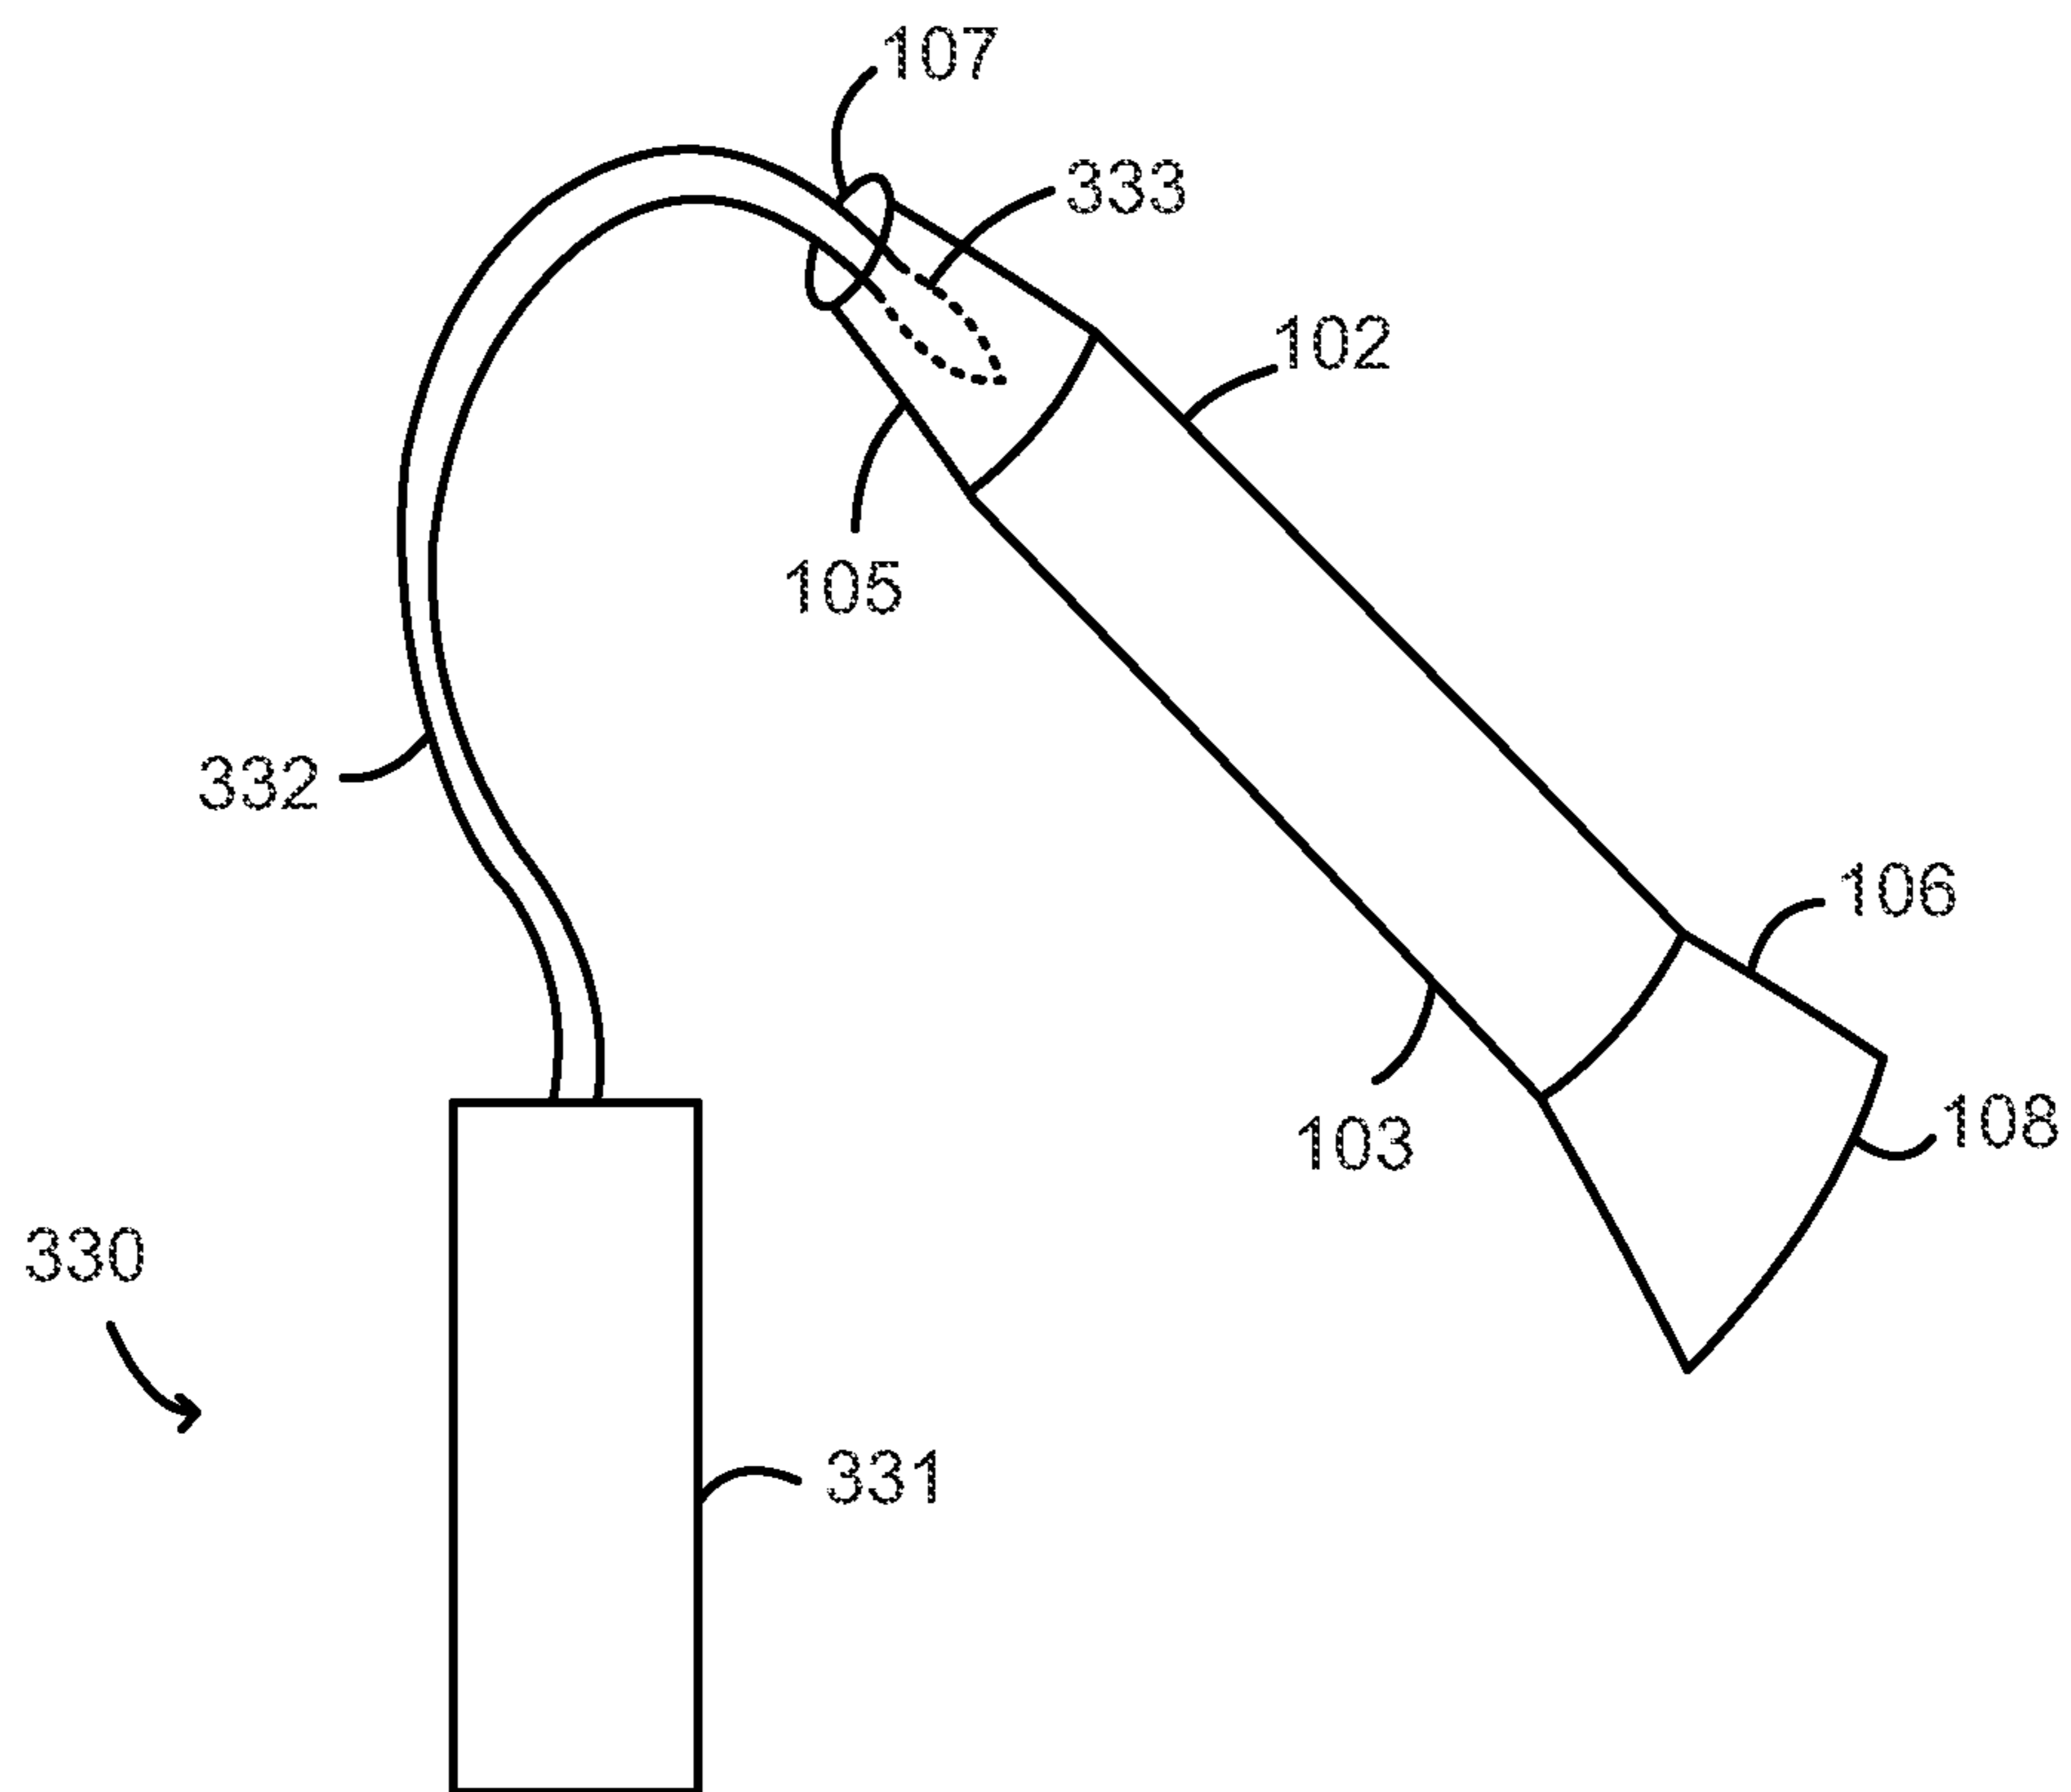


FIG. 3

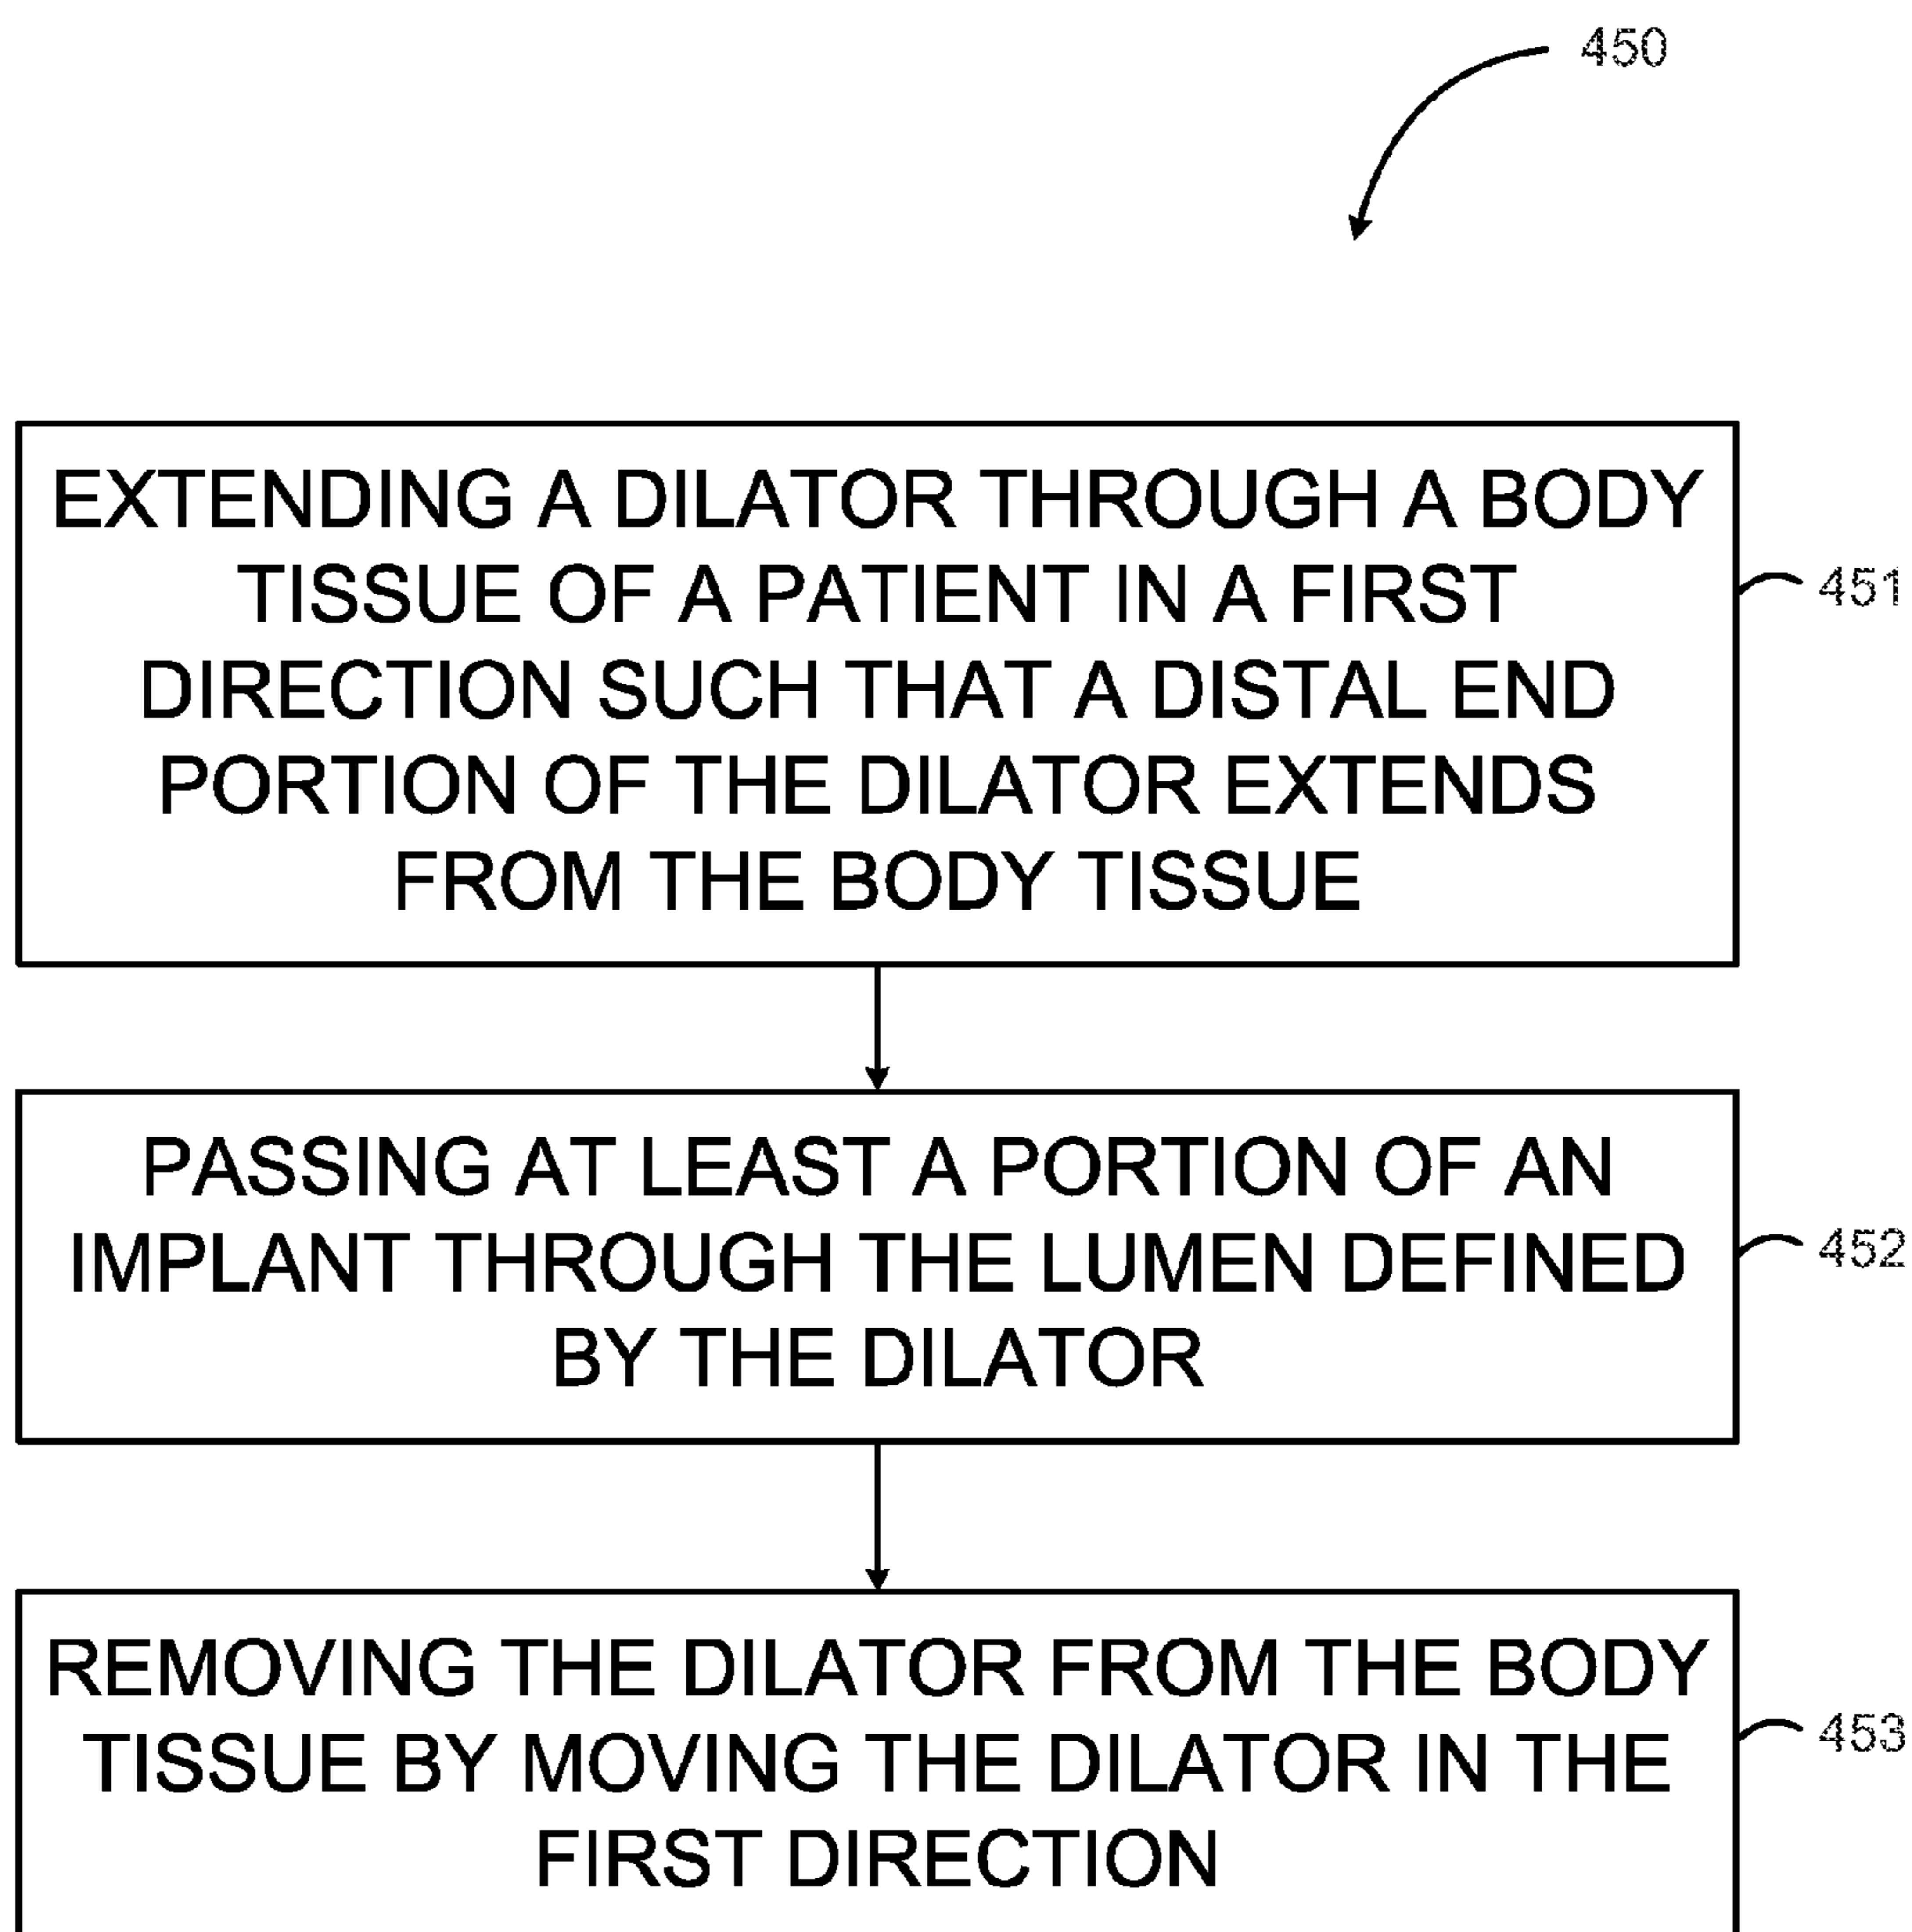


FIG. 4



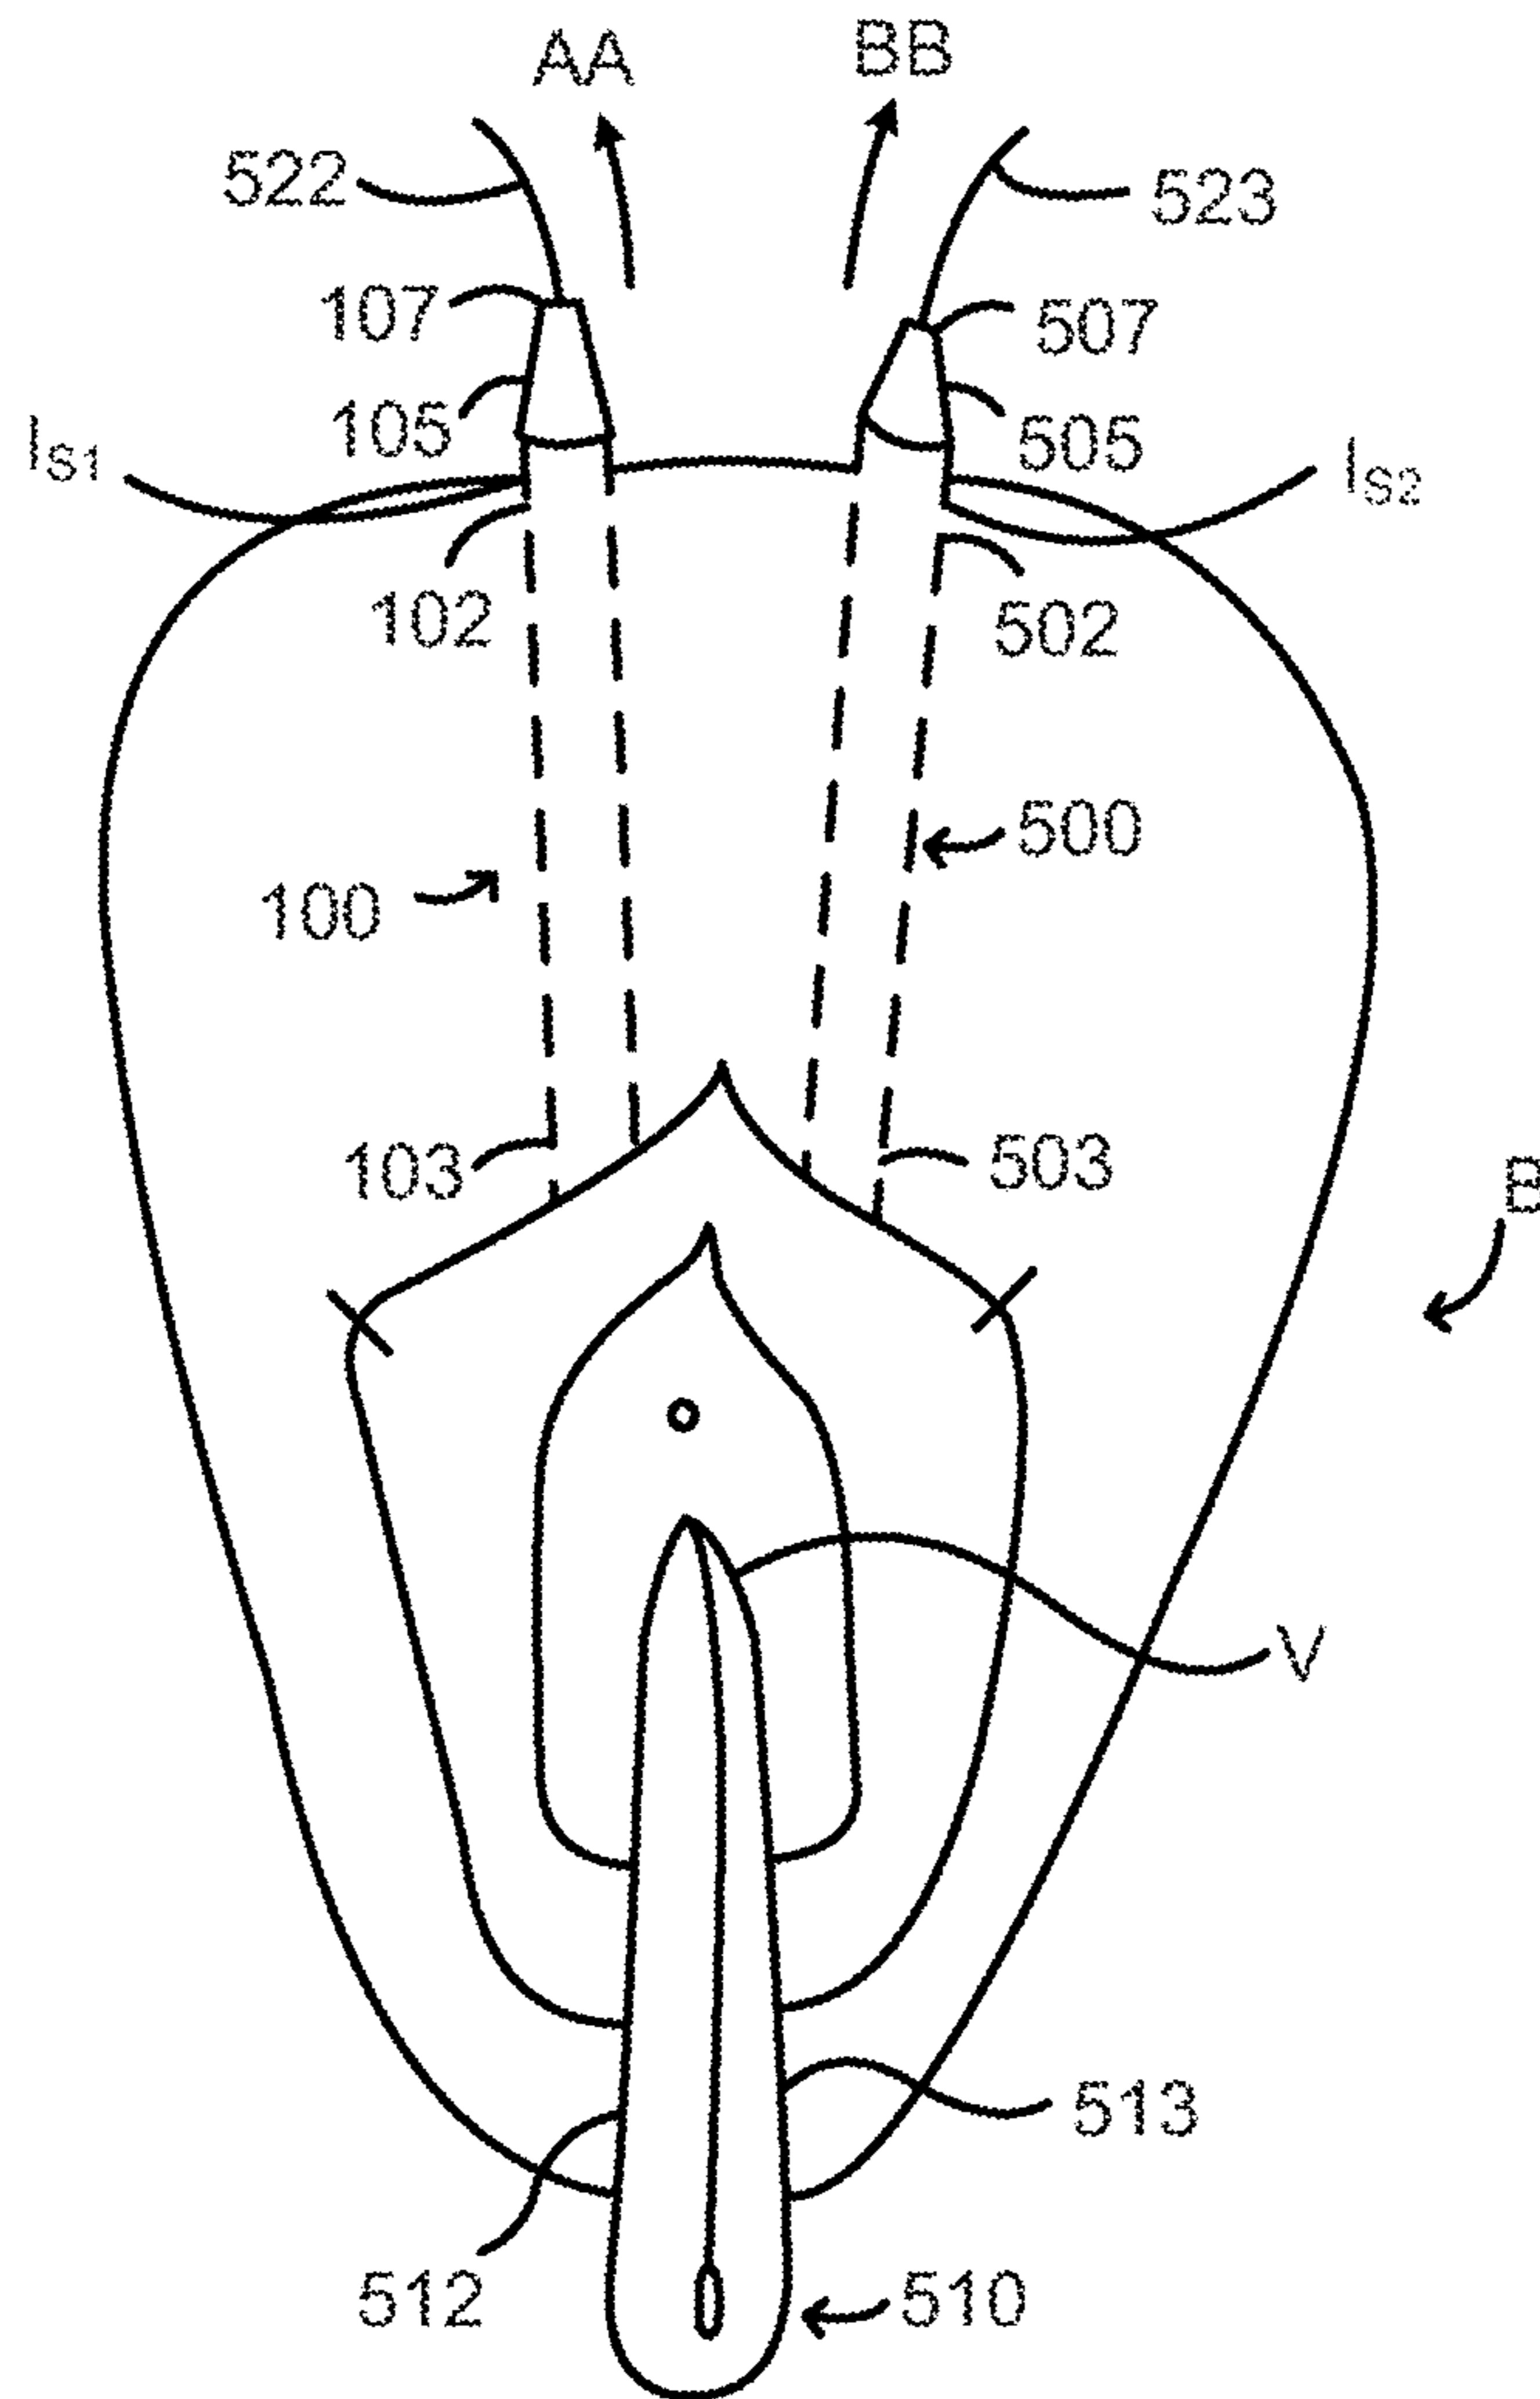


FIG. 5

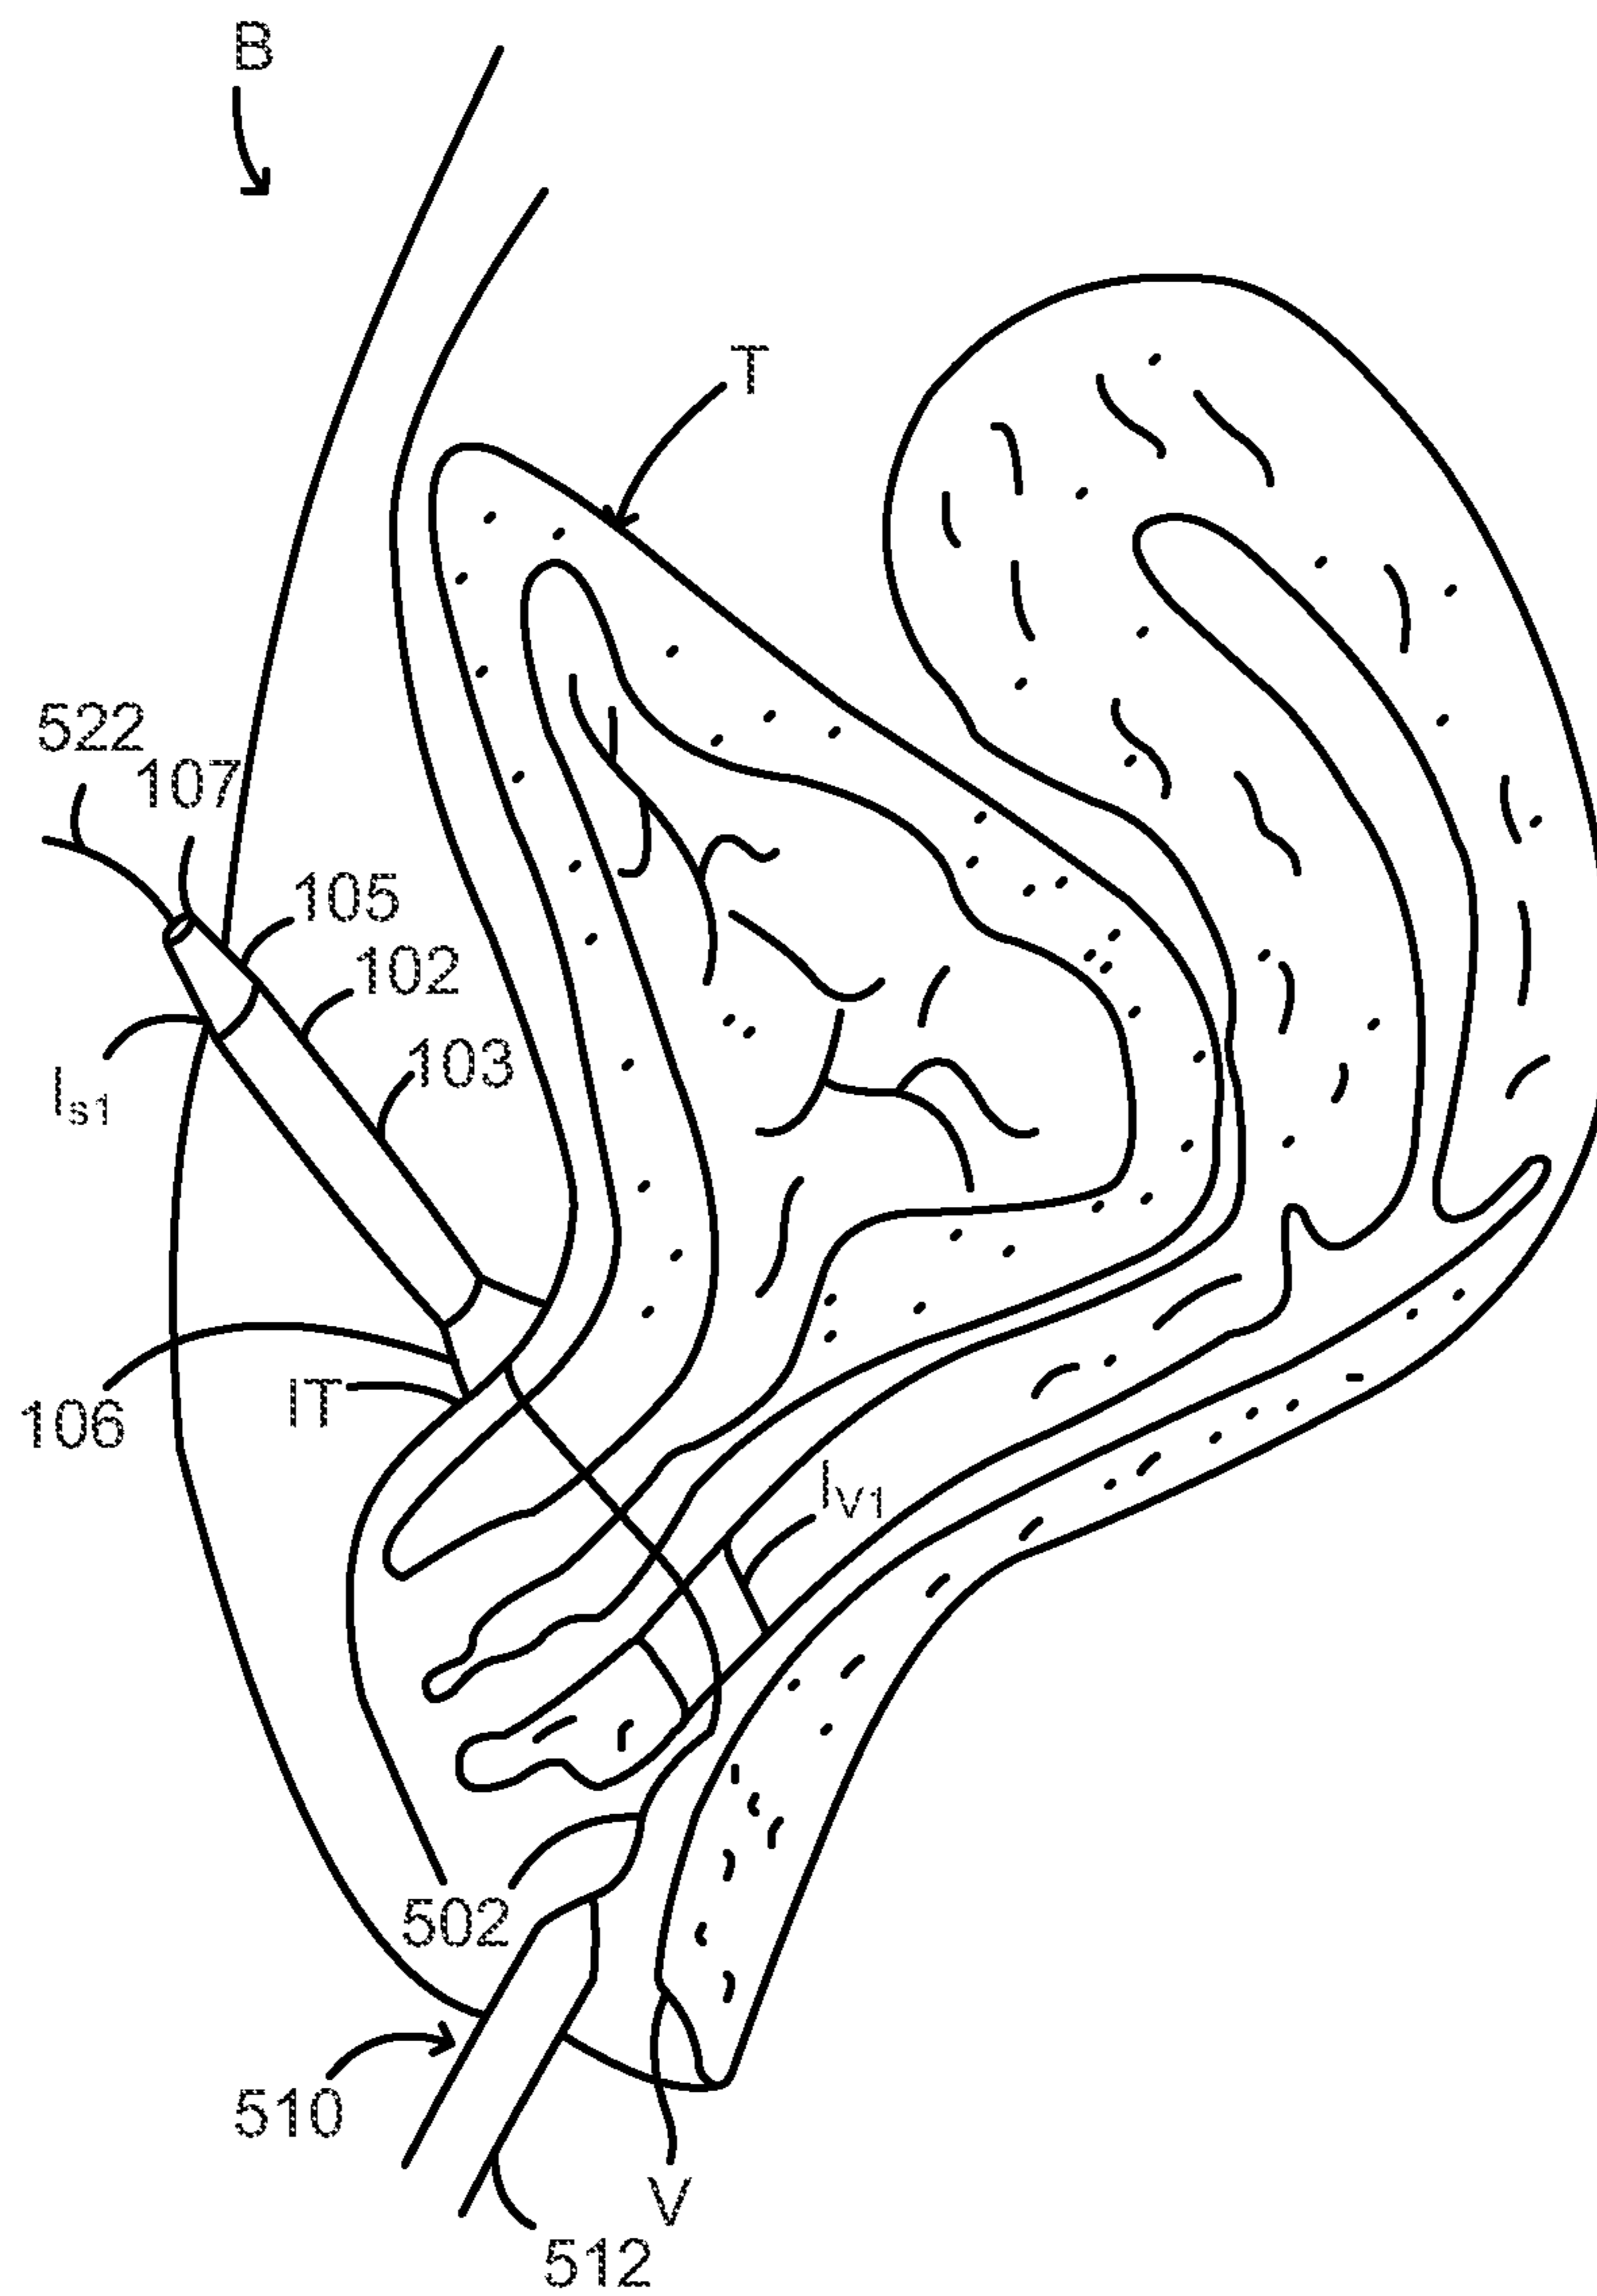


FIG. 6

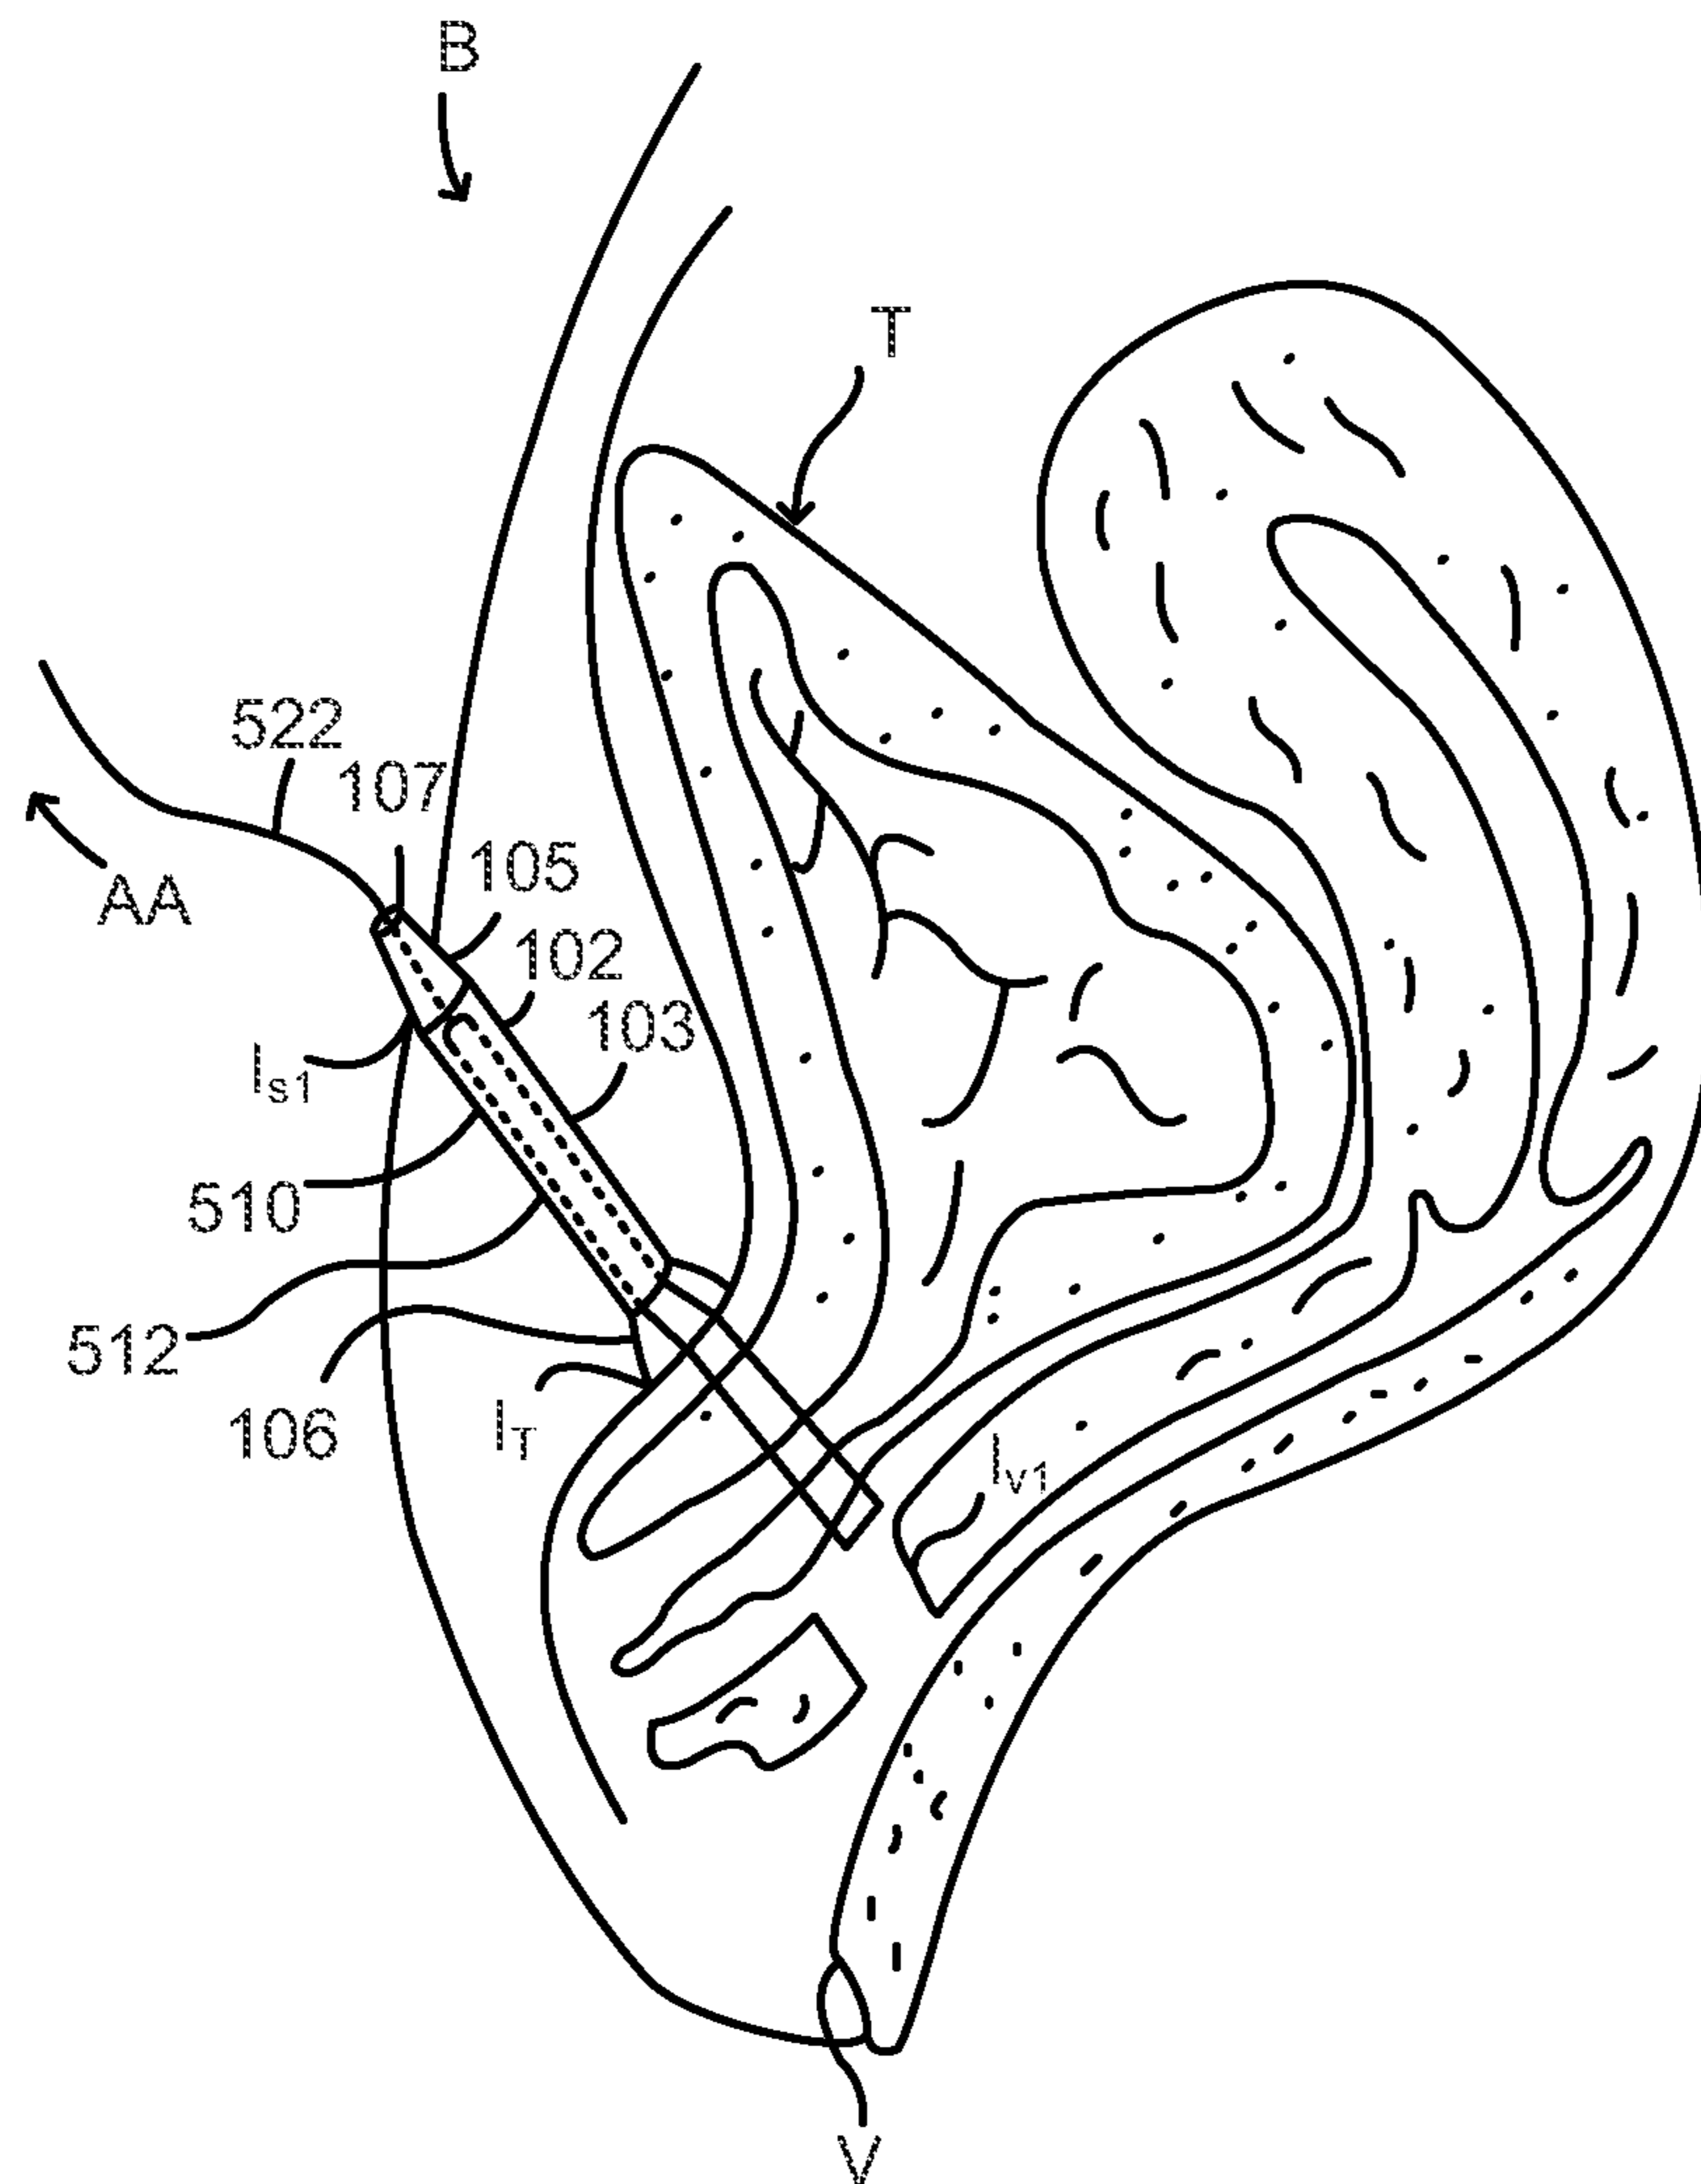


FIG. 7

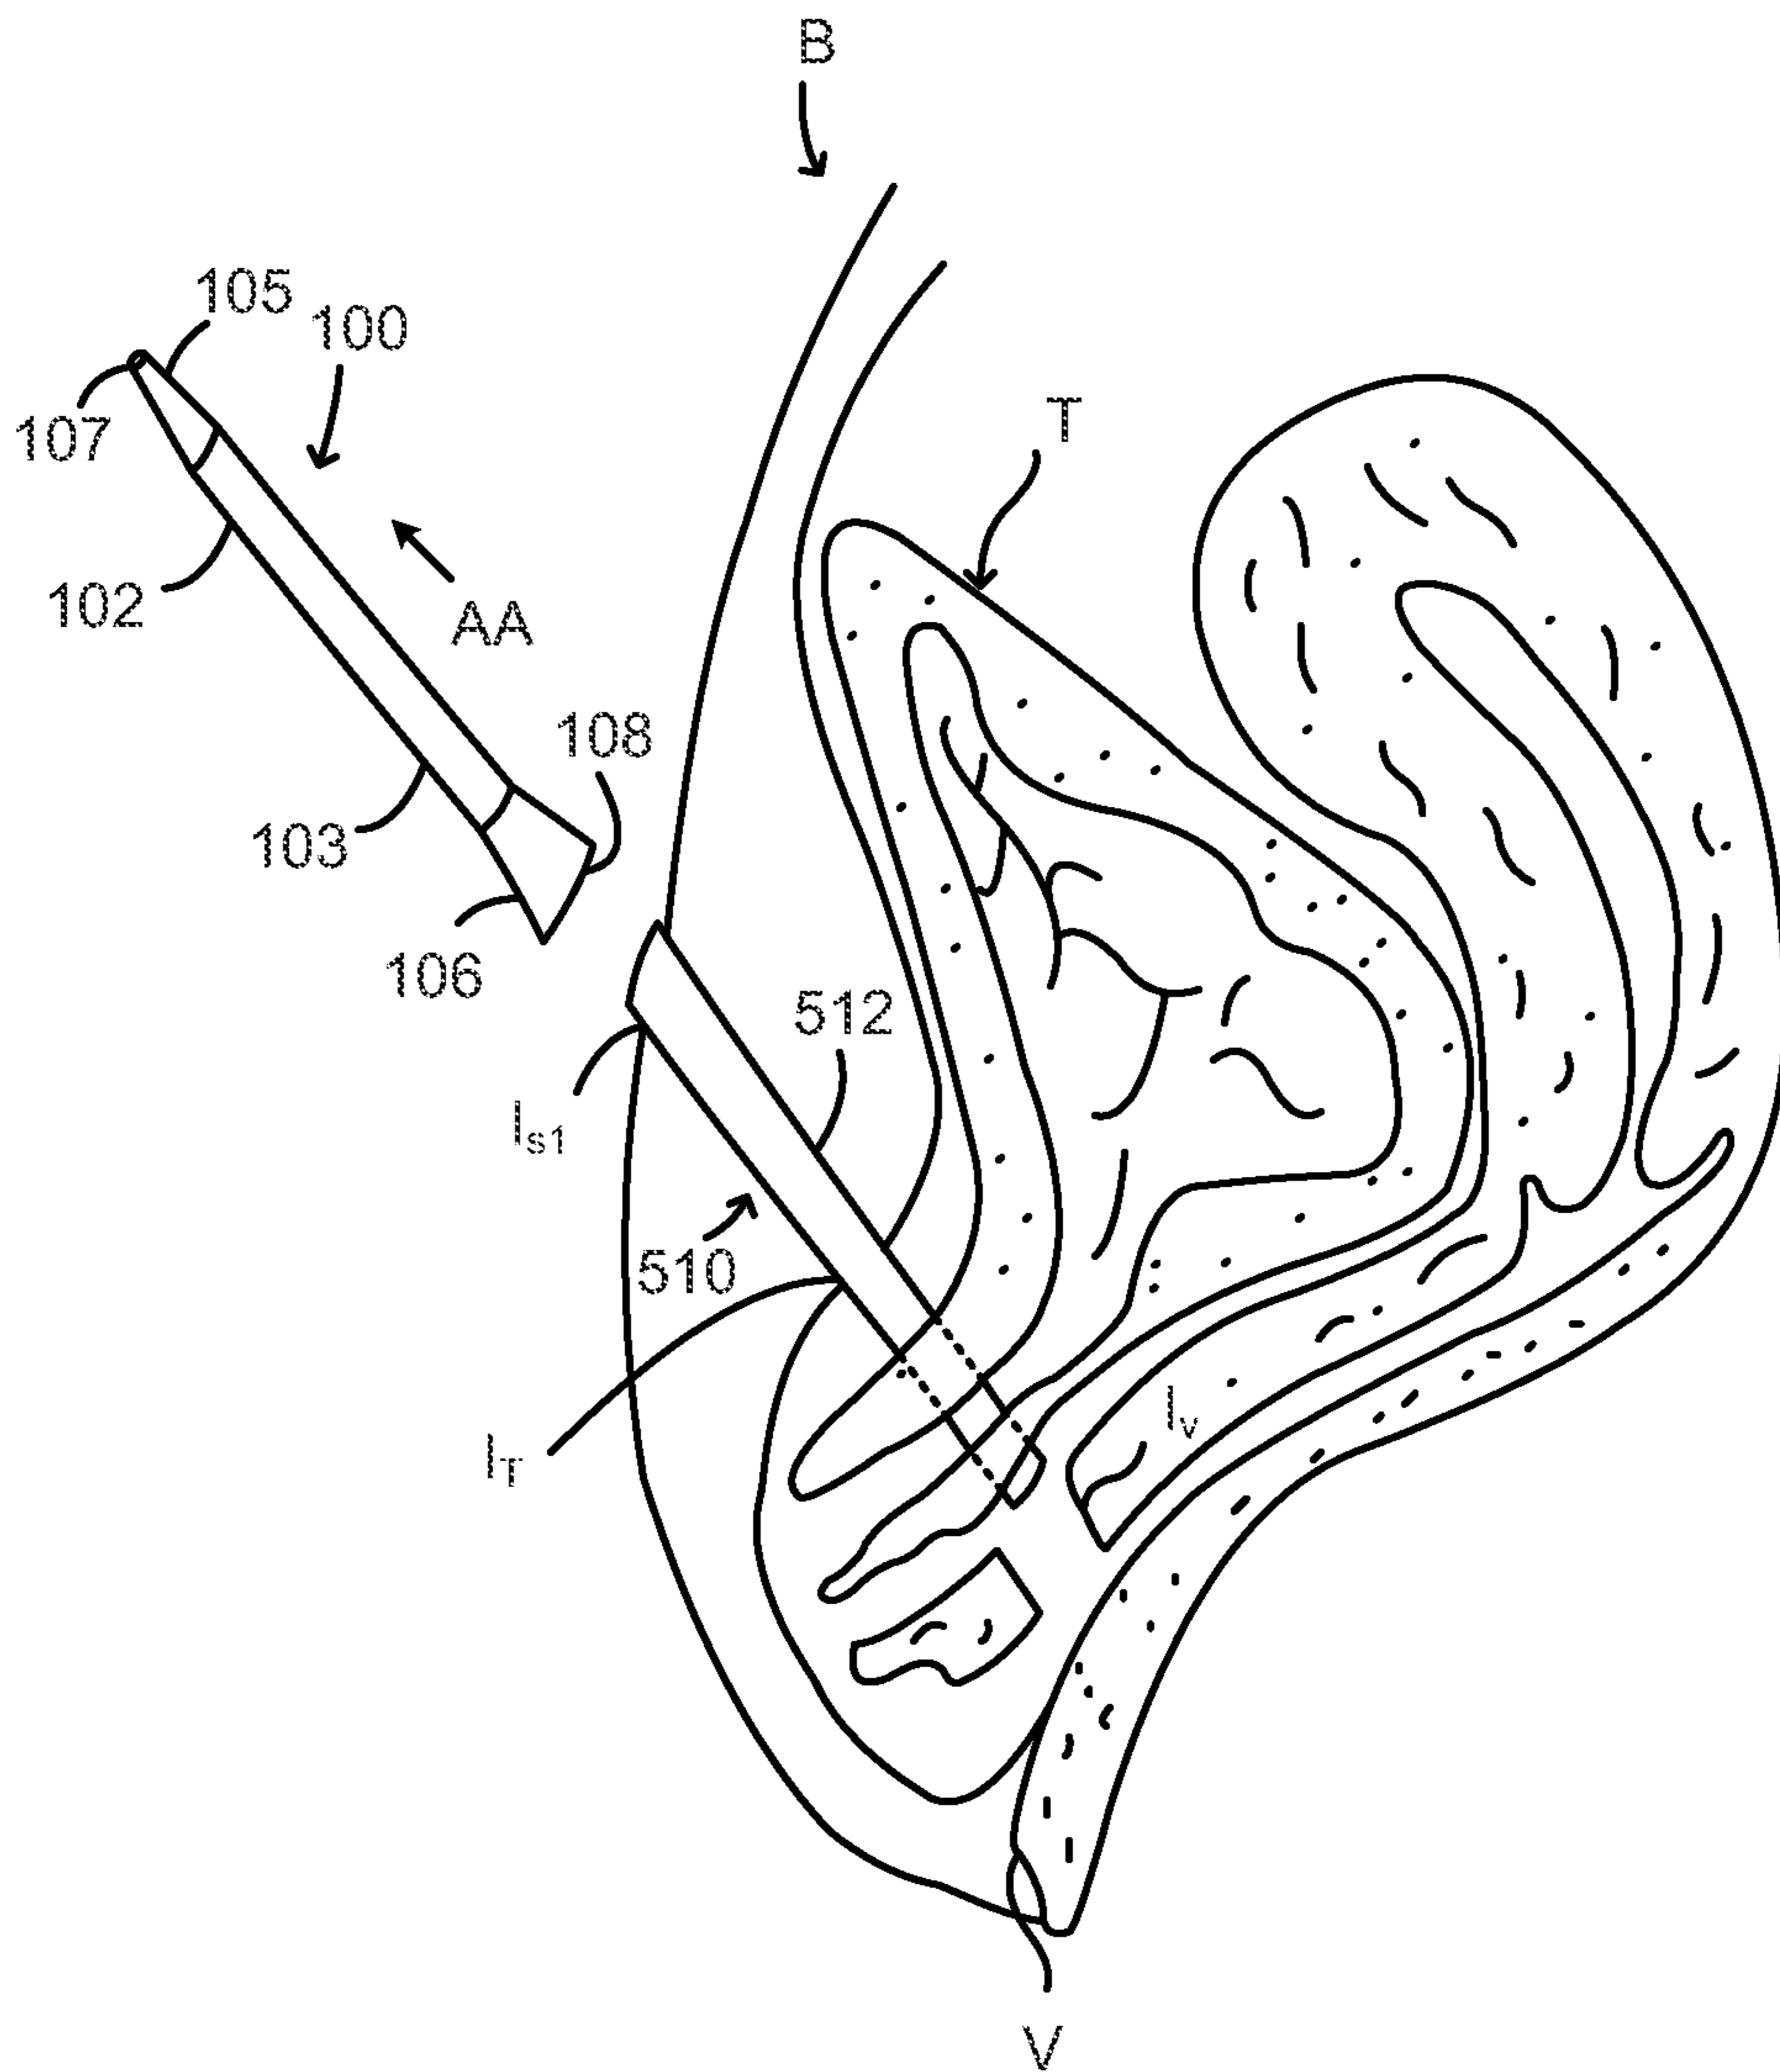


FIG. 8

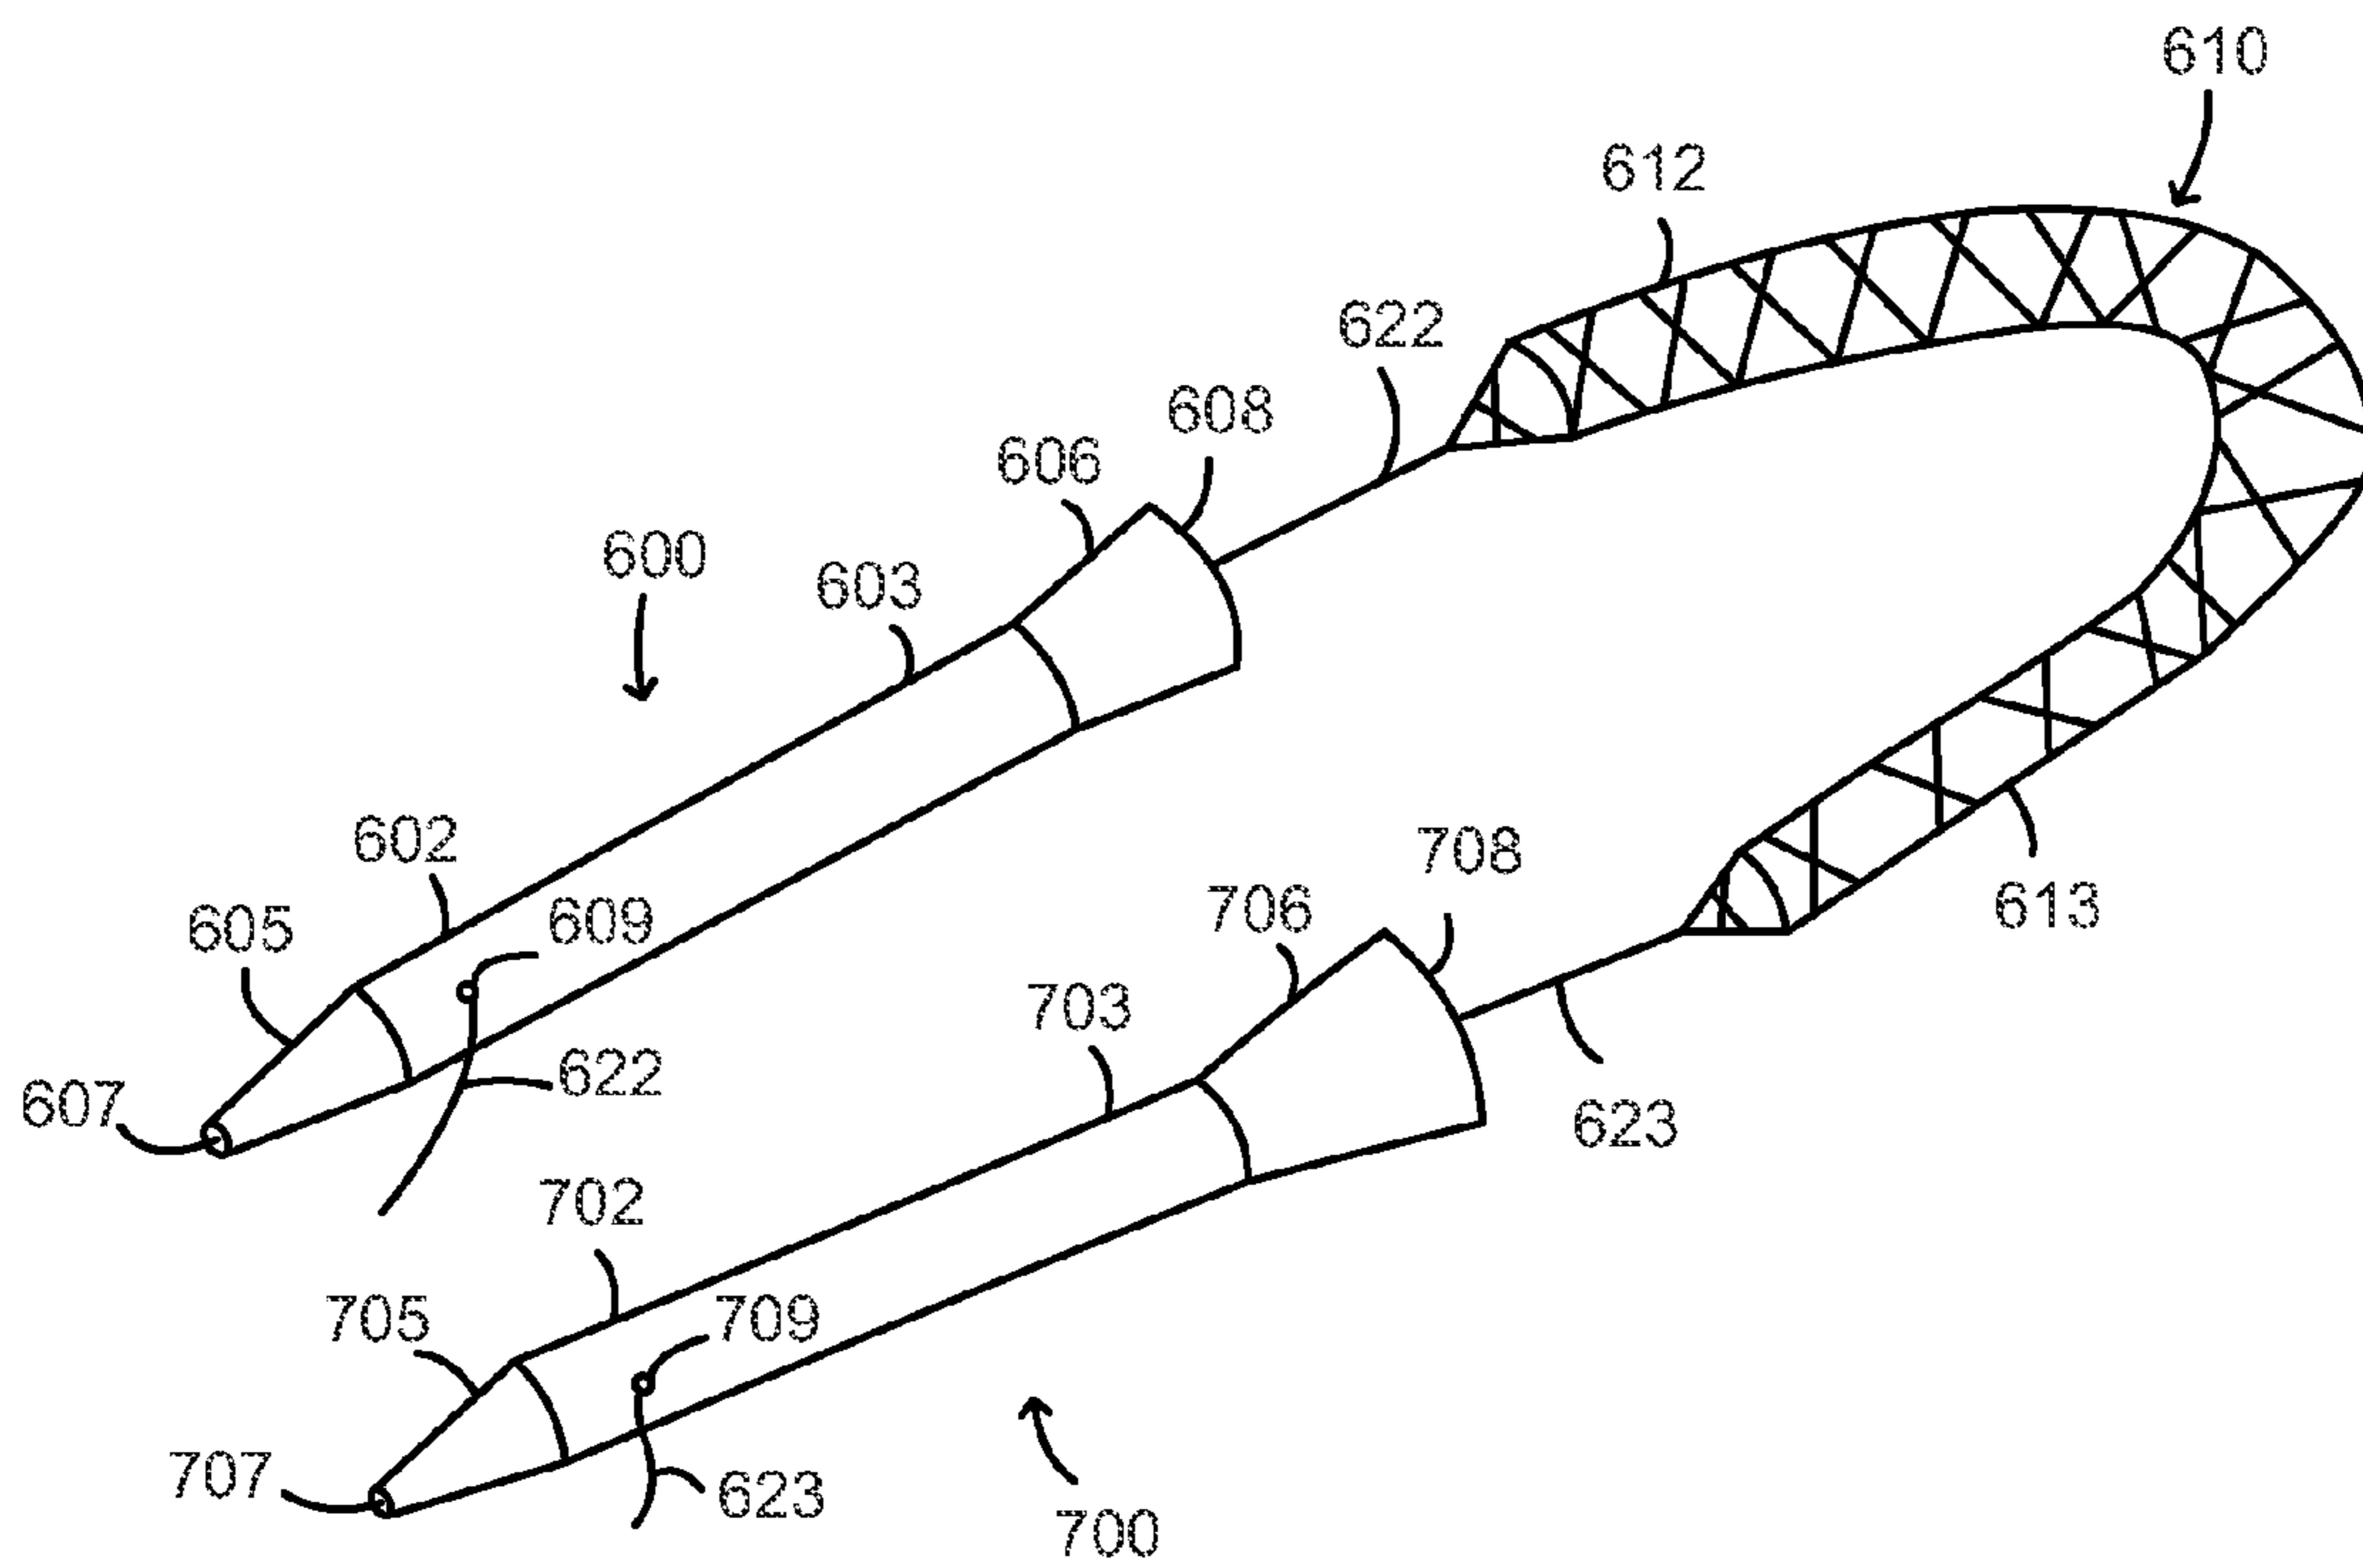


FIG. 9

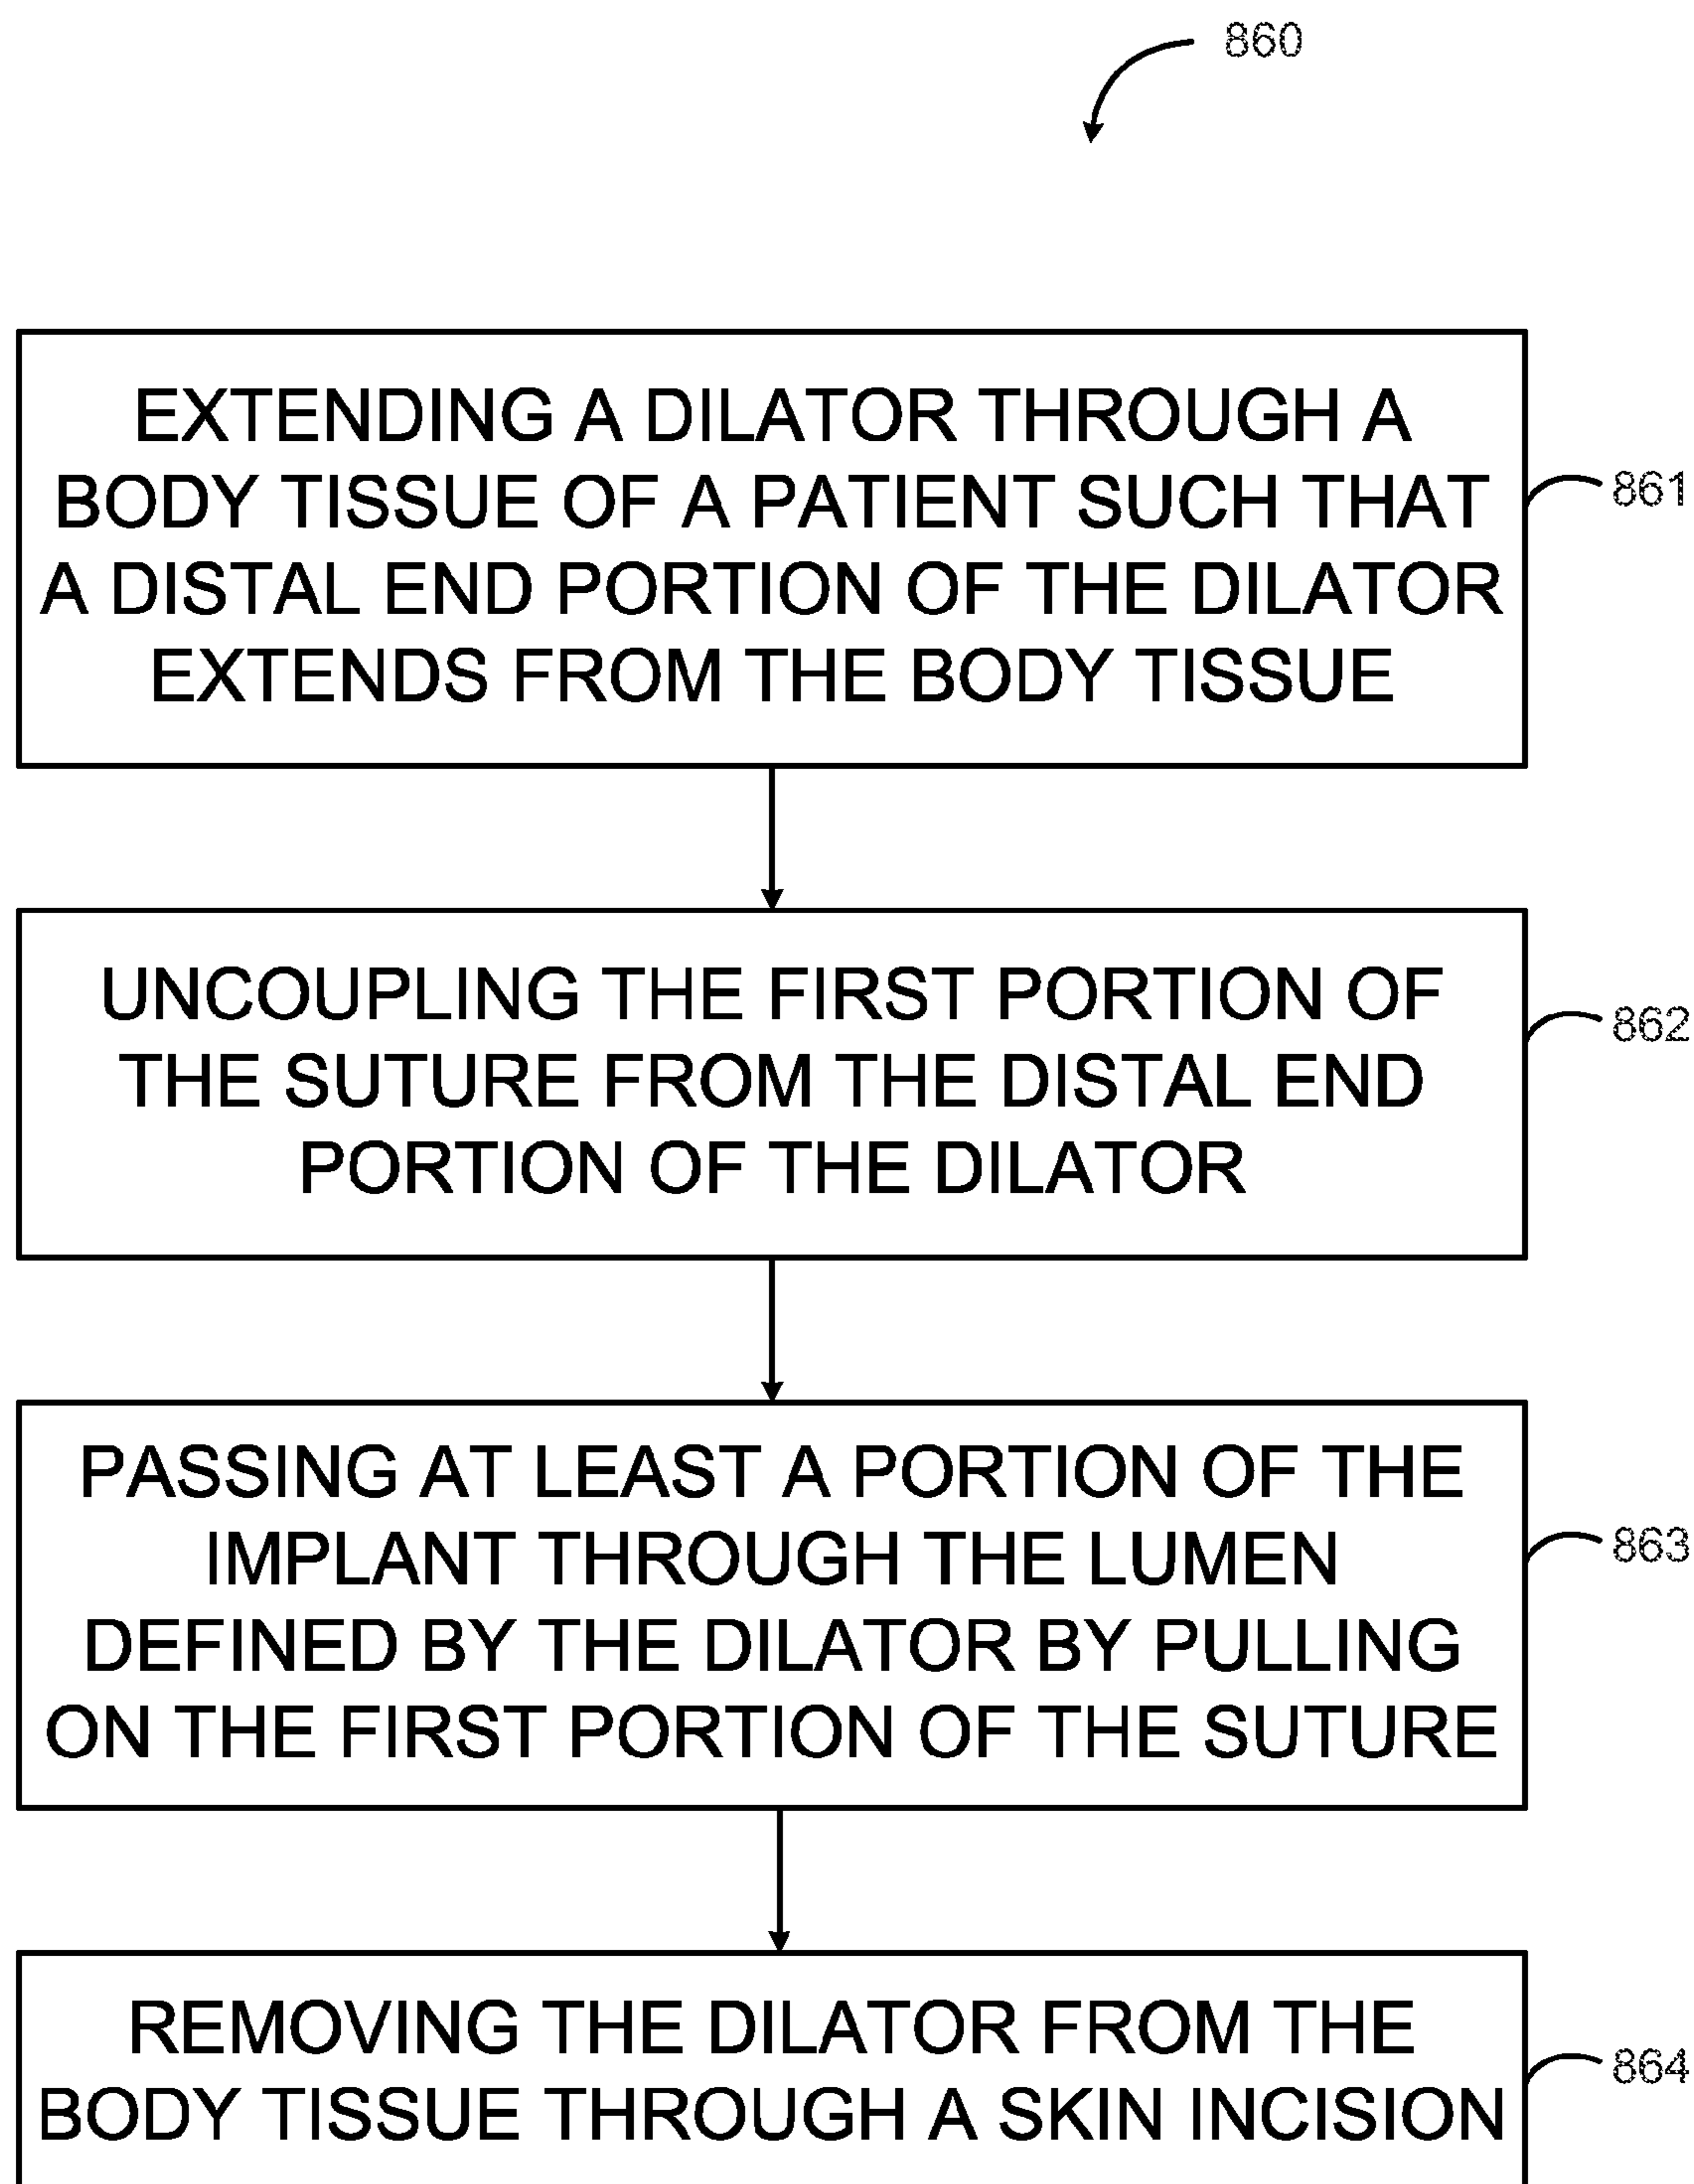


FIG. 10

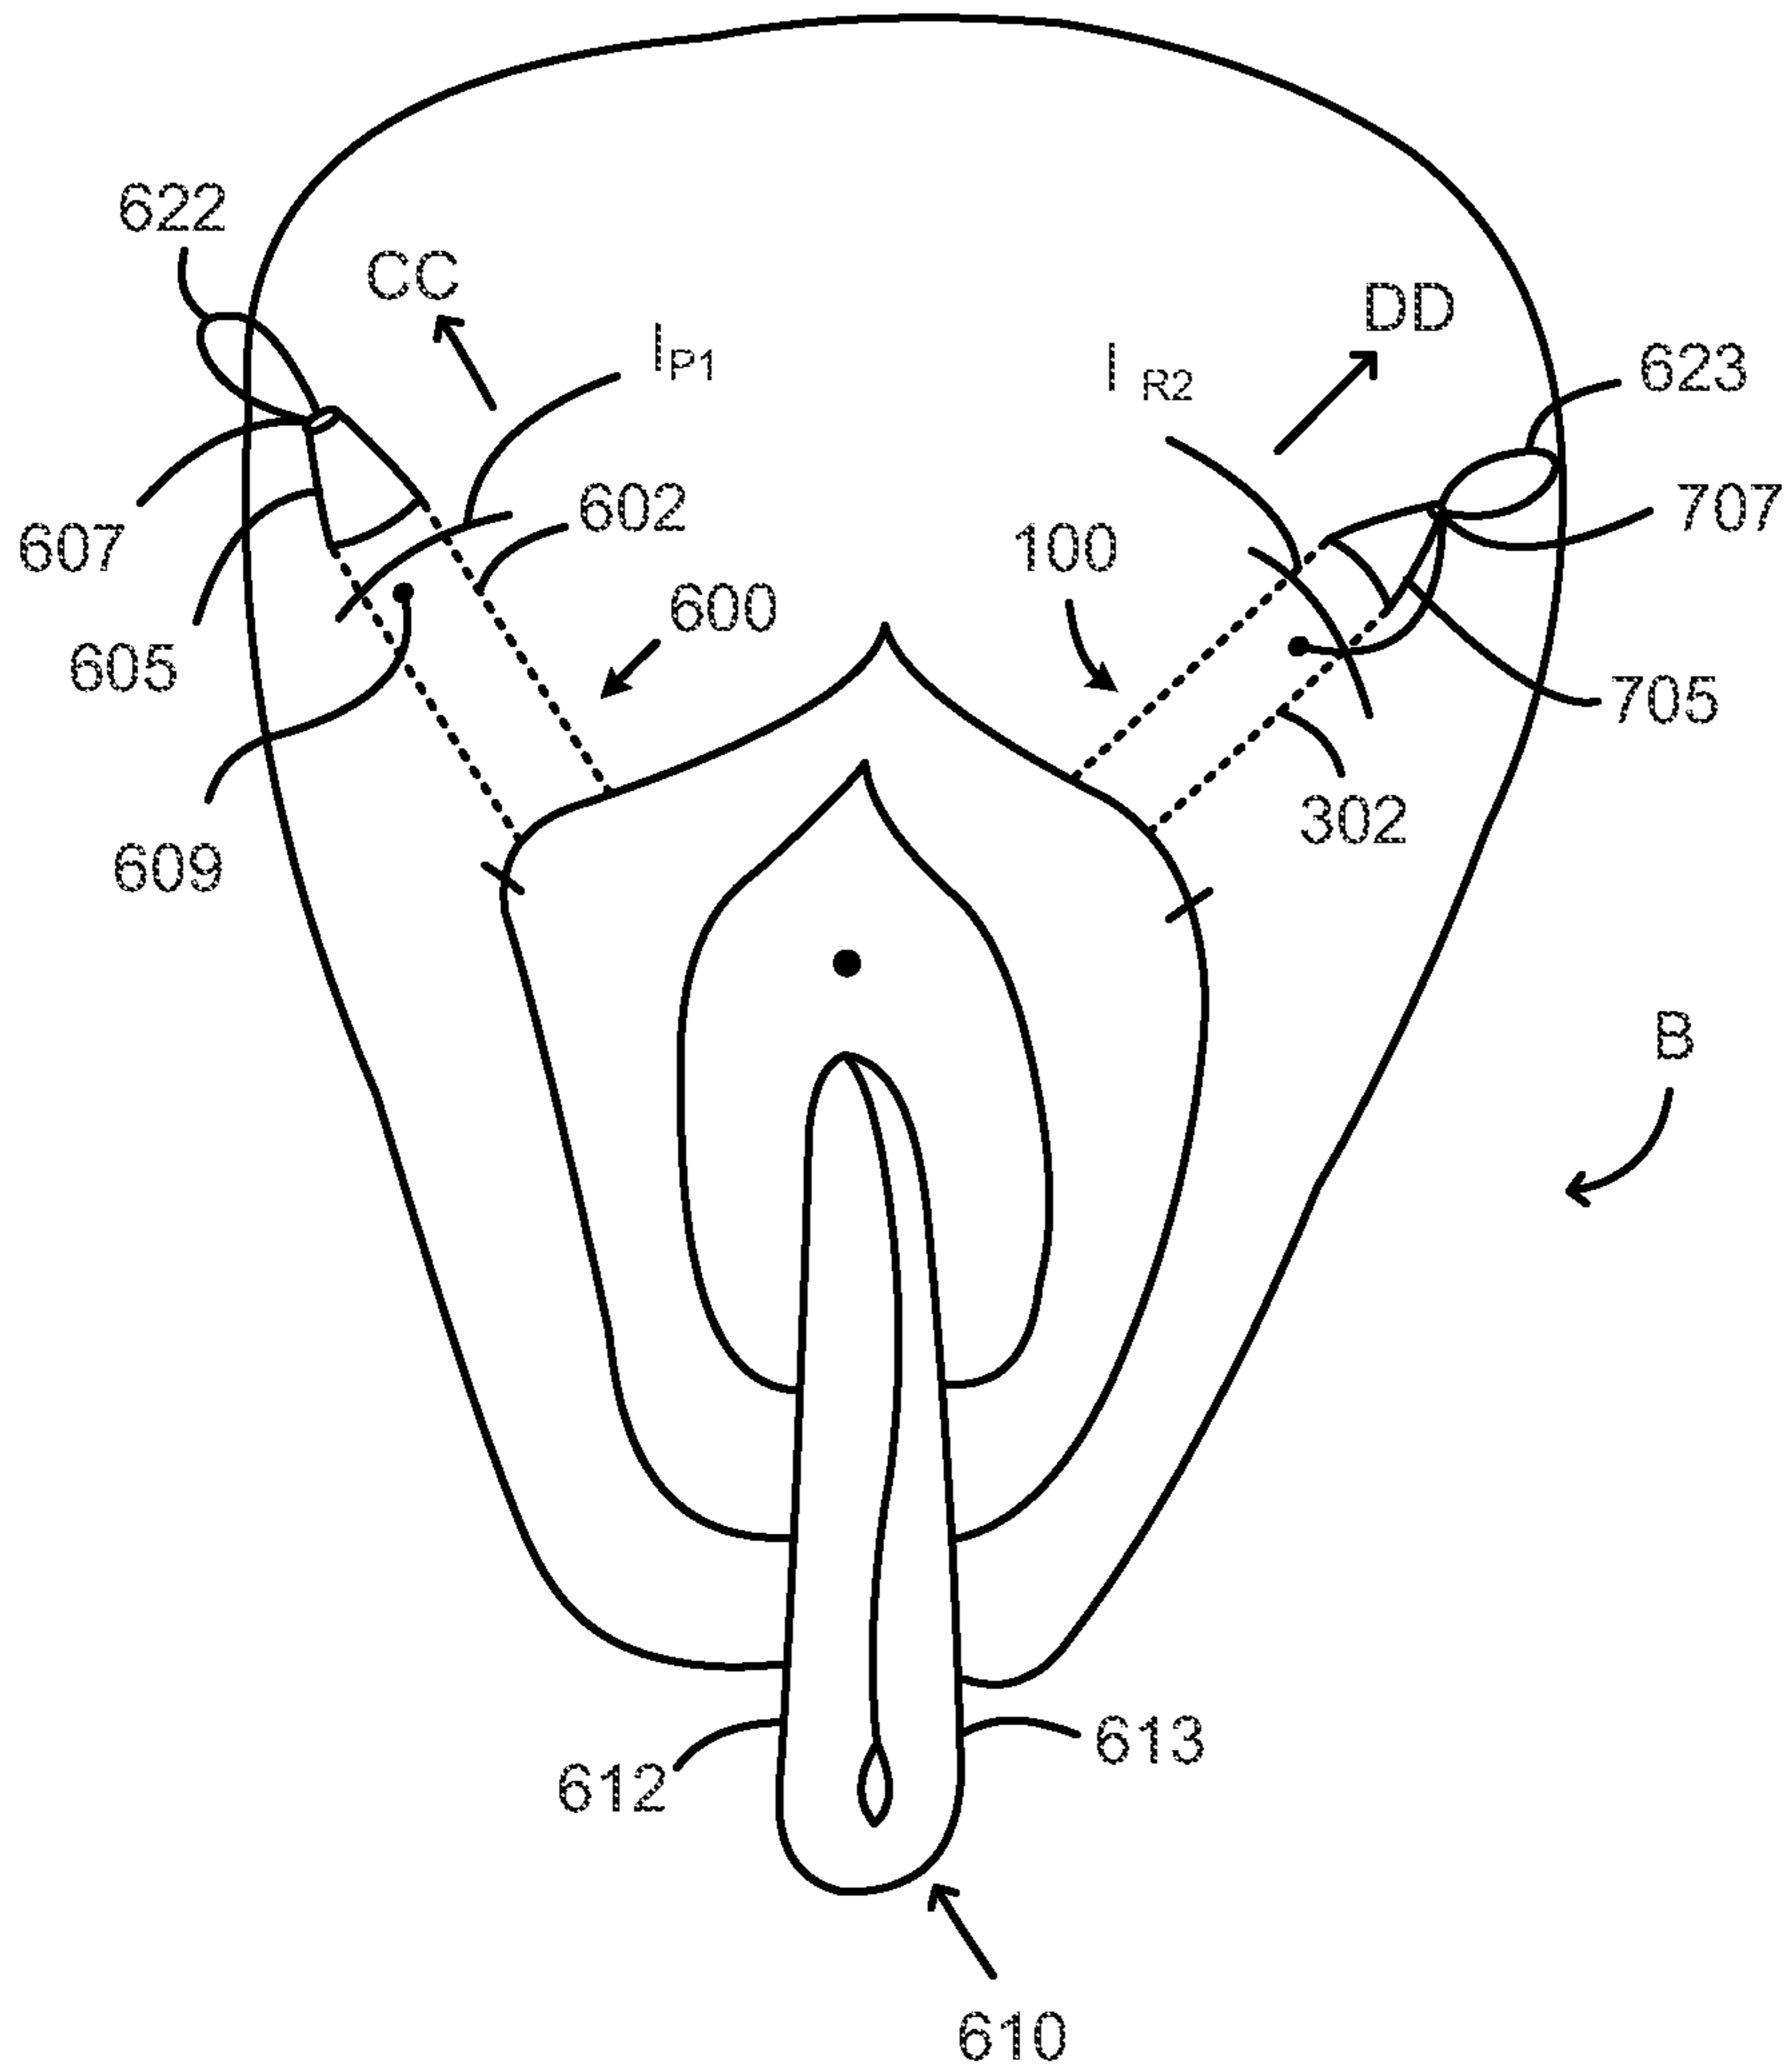


FIG. 11

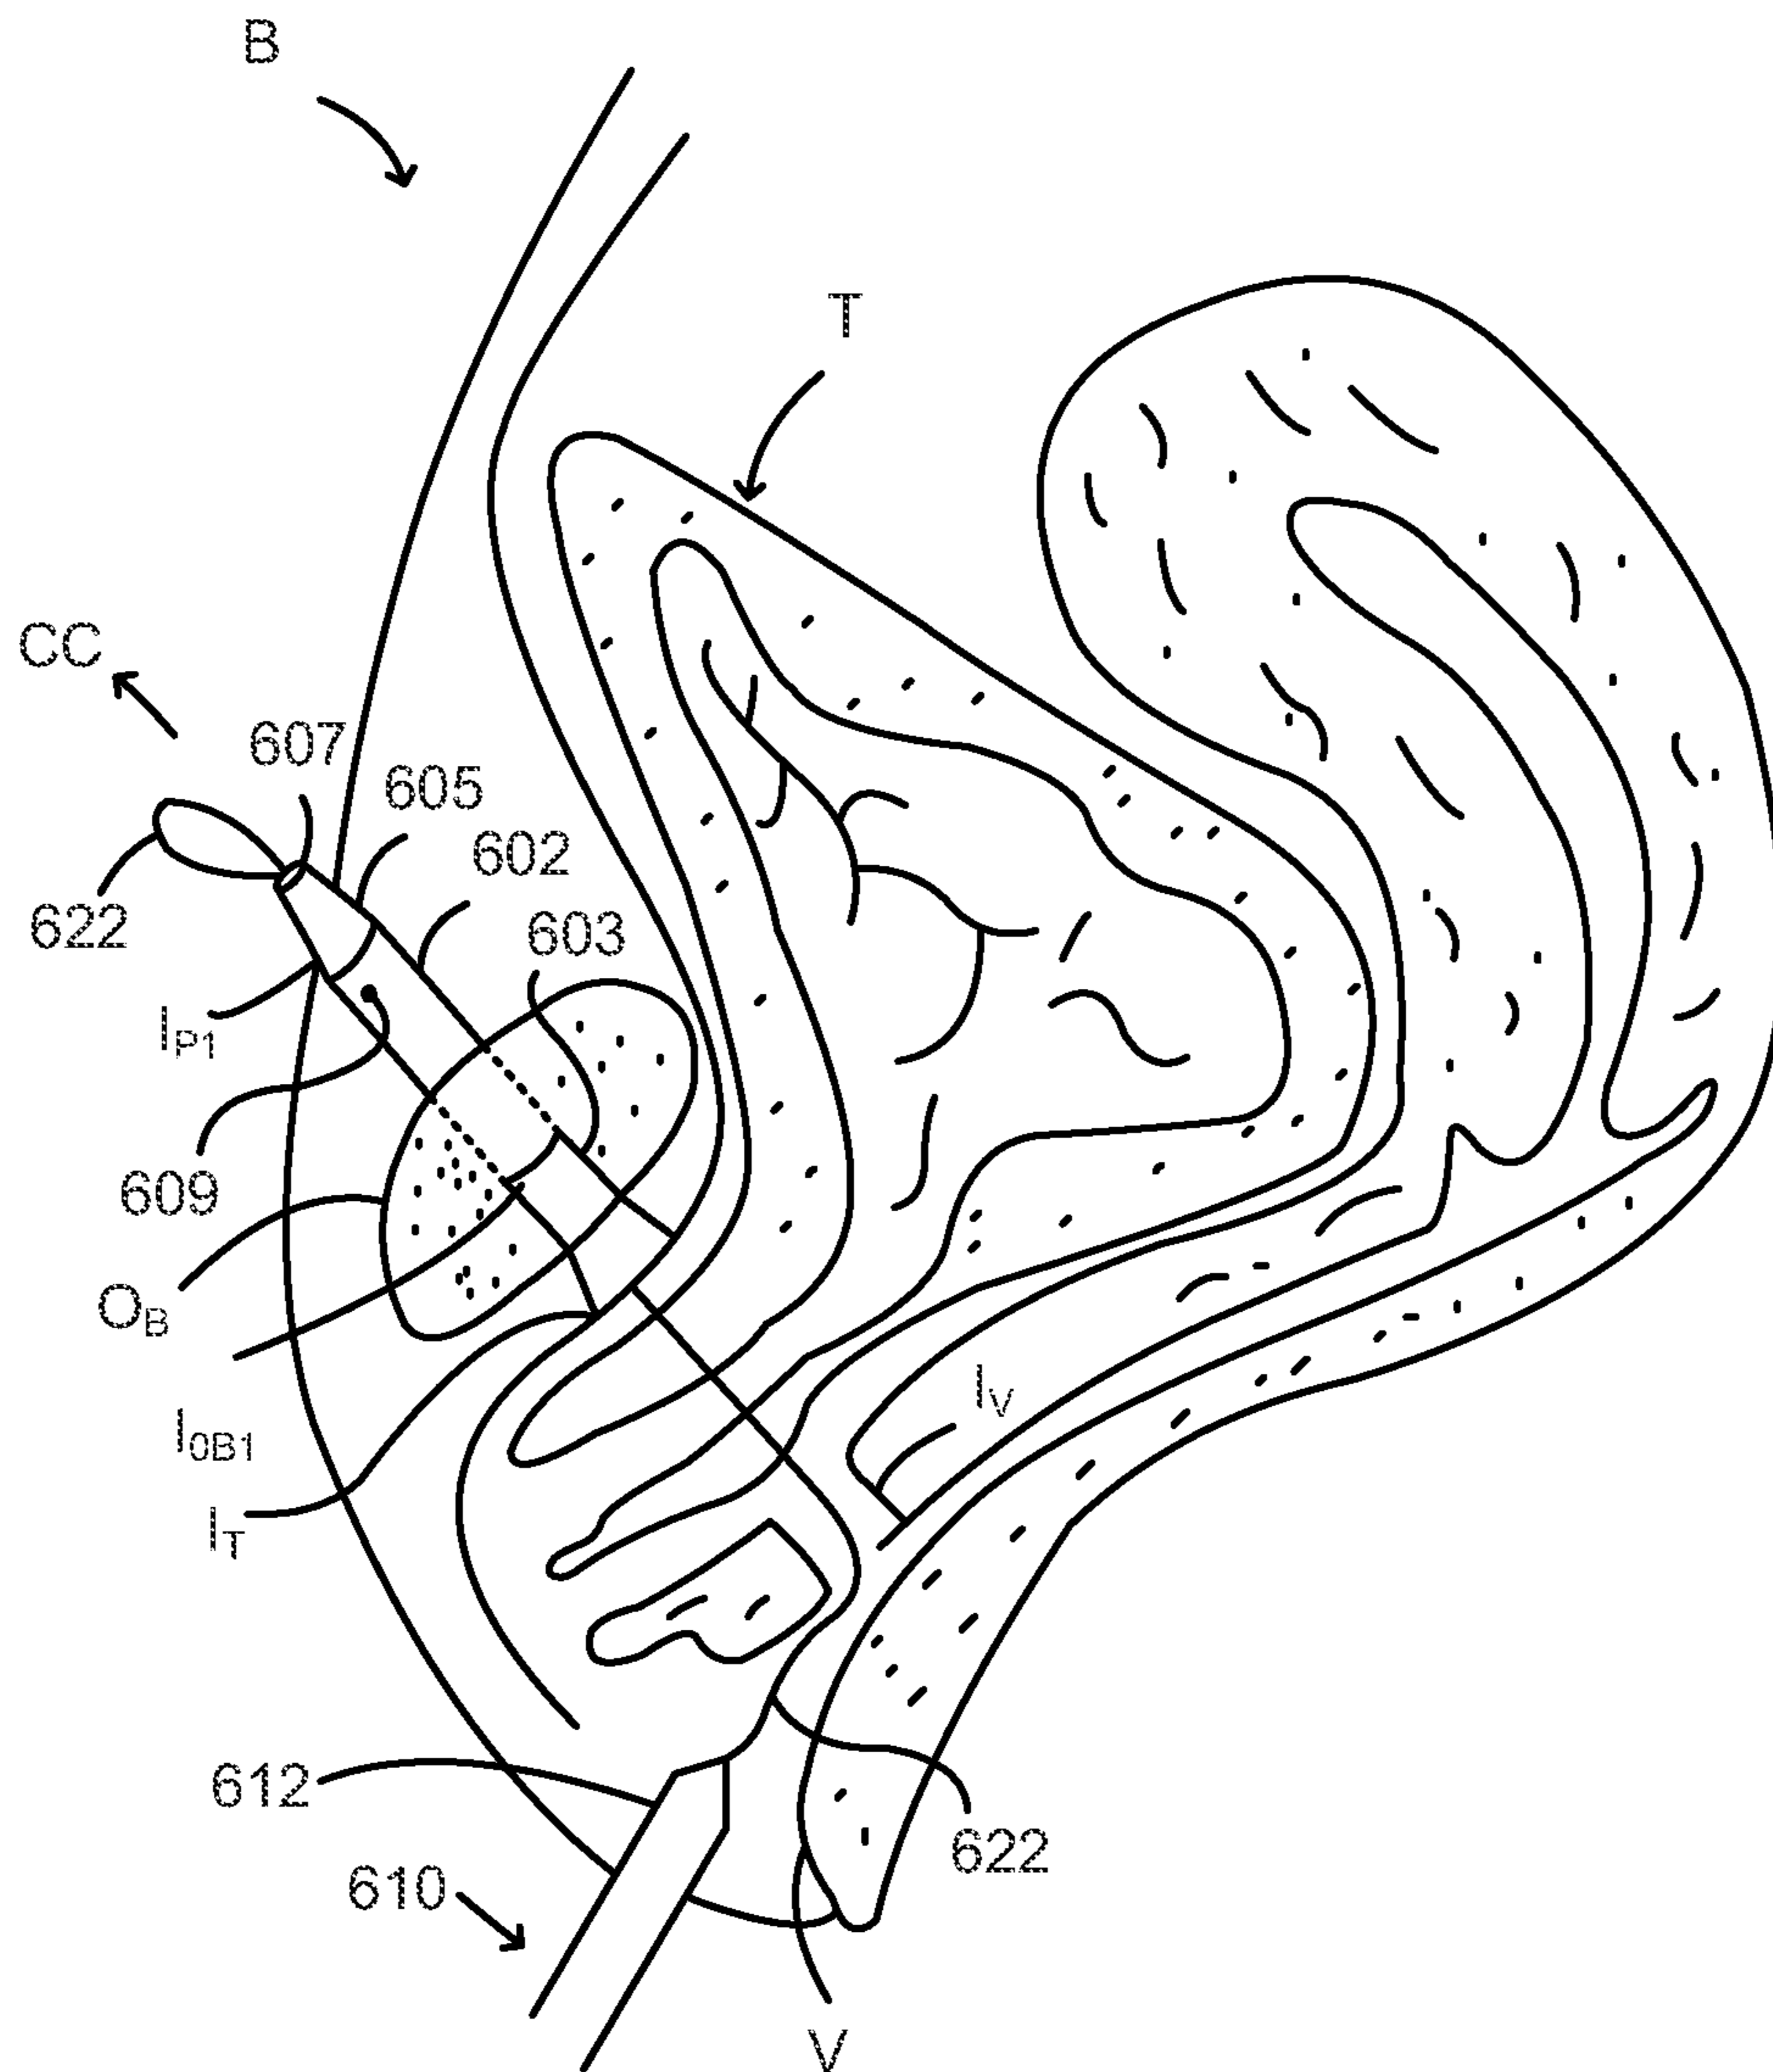


FIG. 12



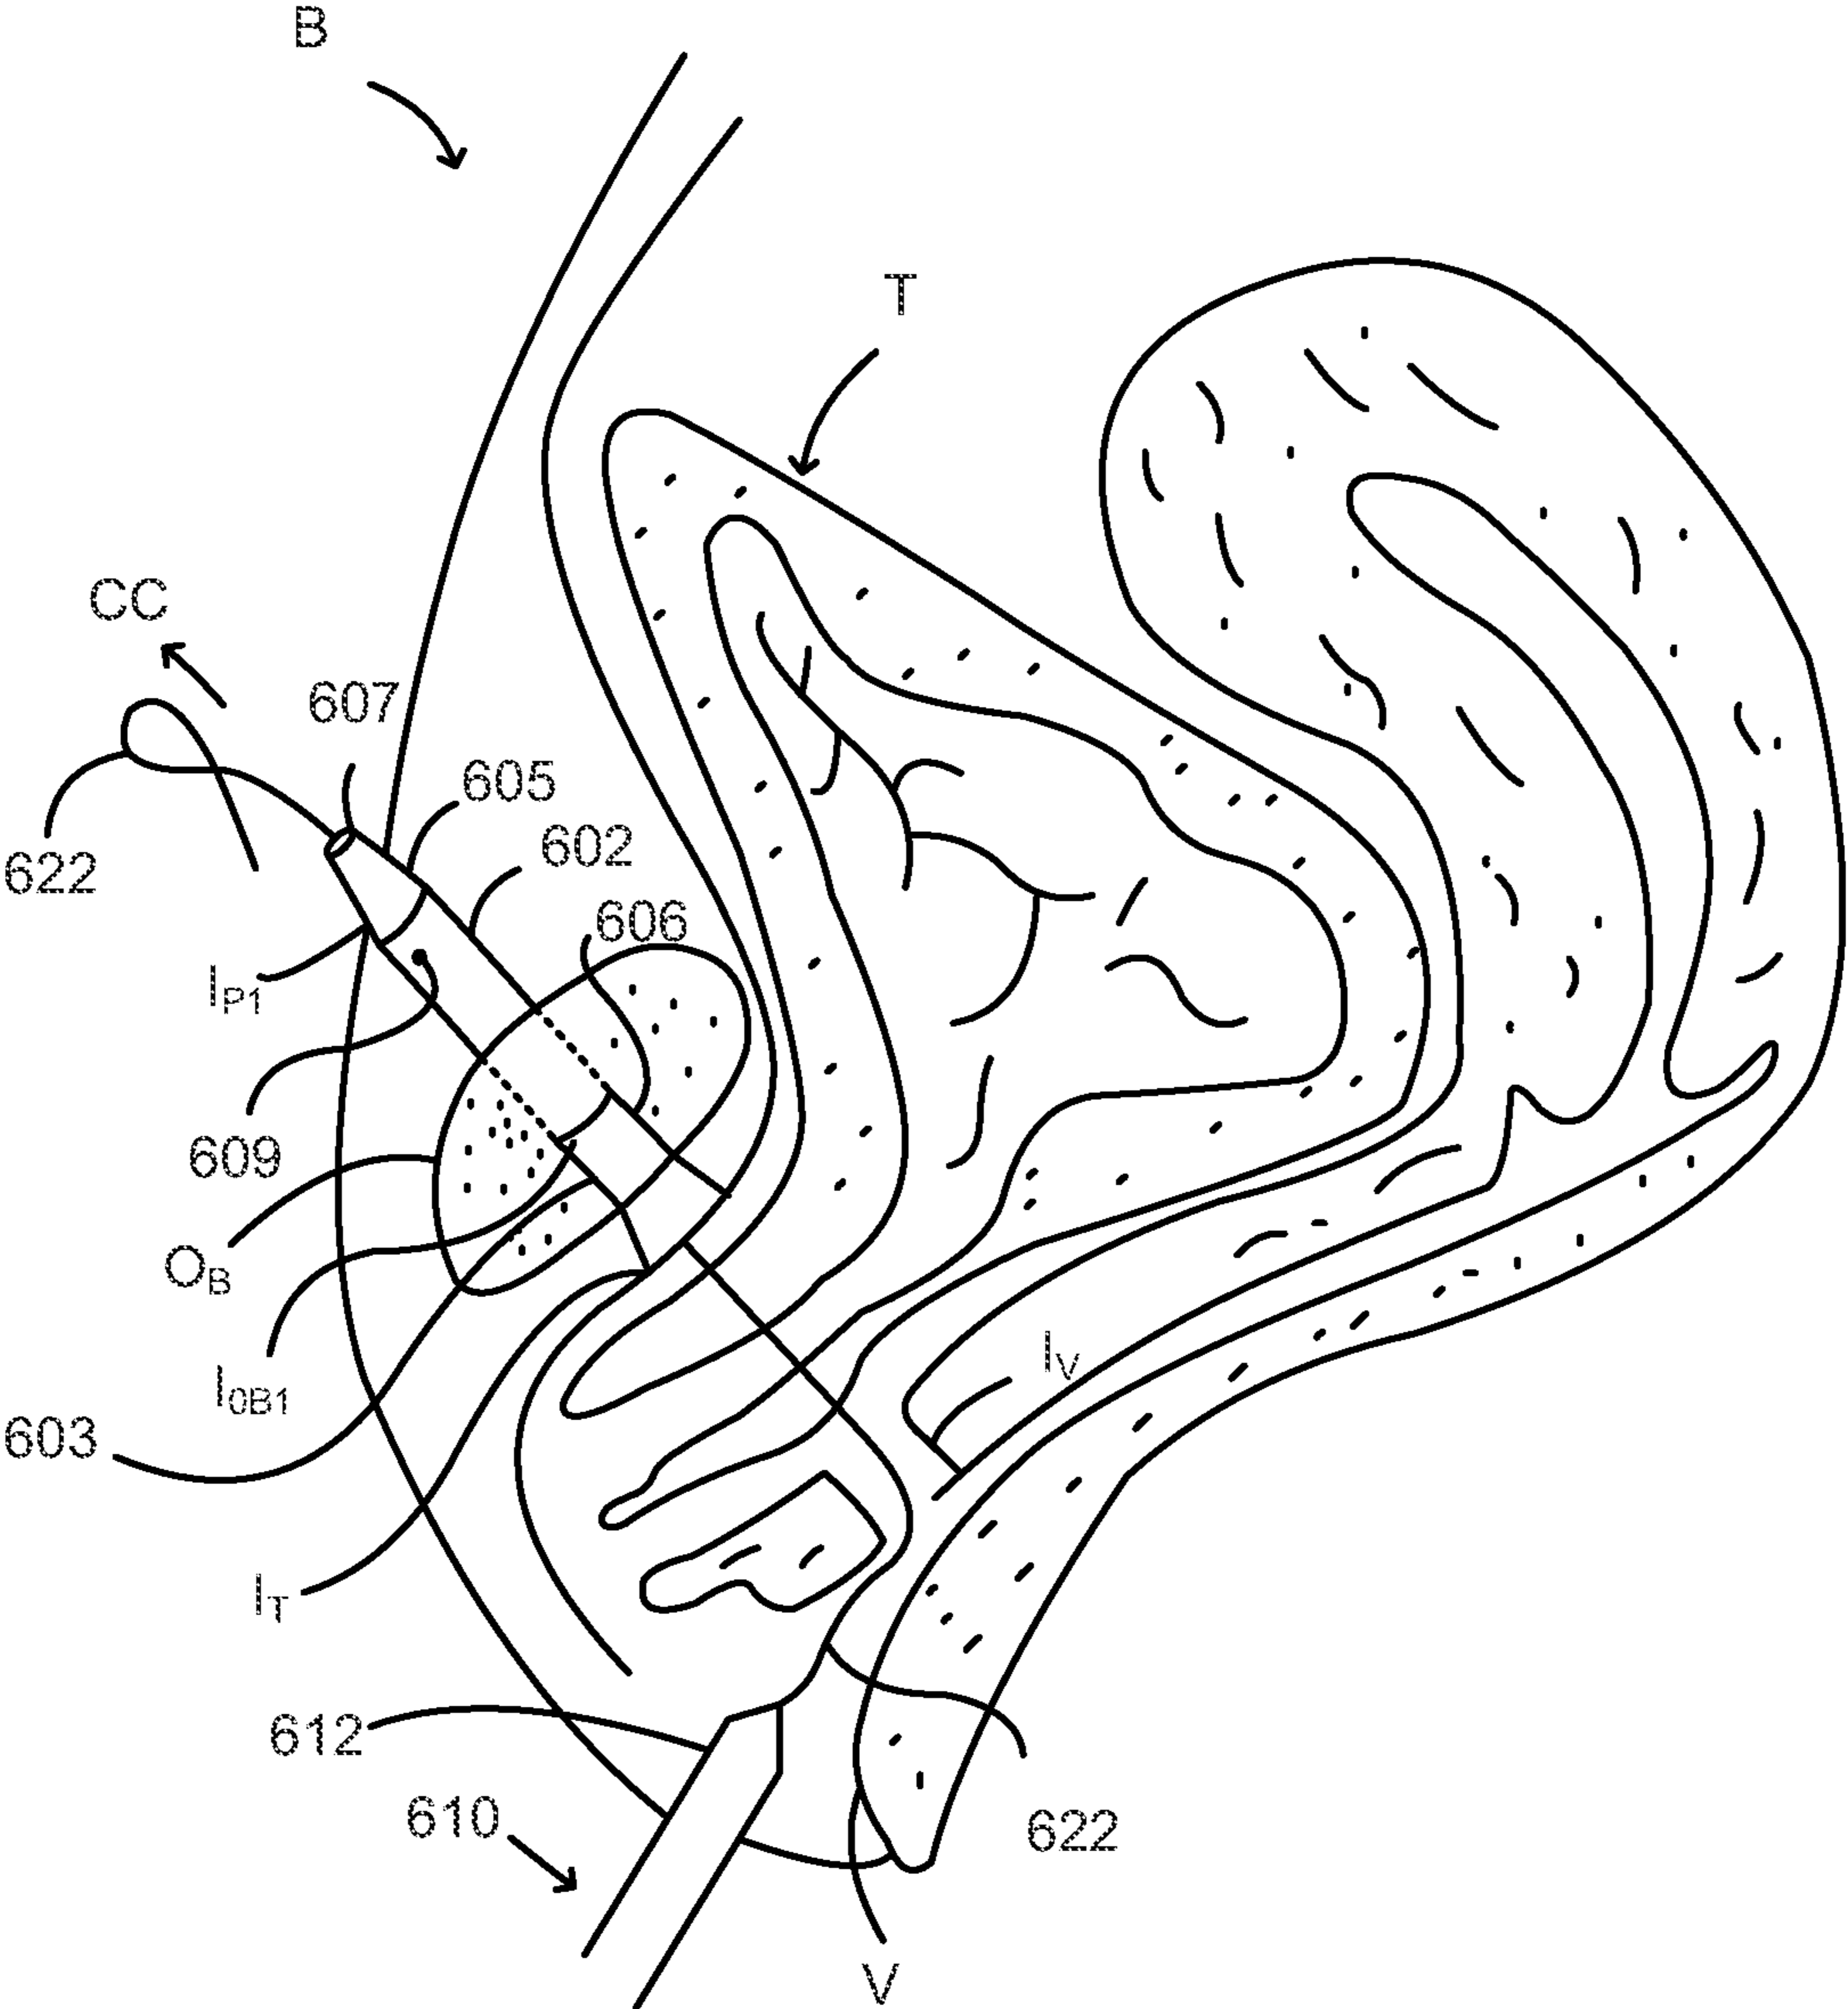


FIG. 13

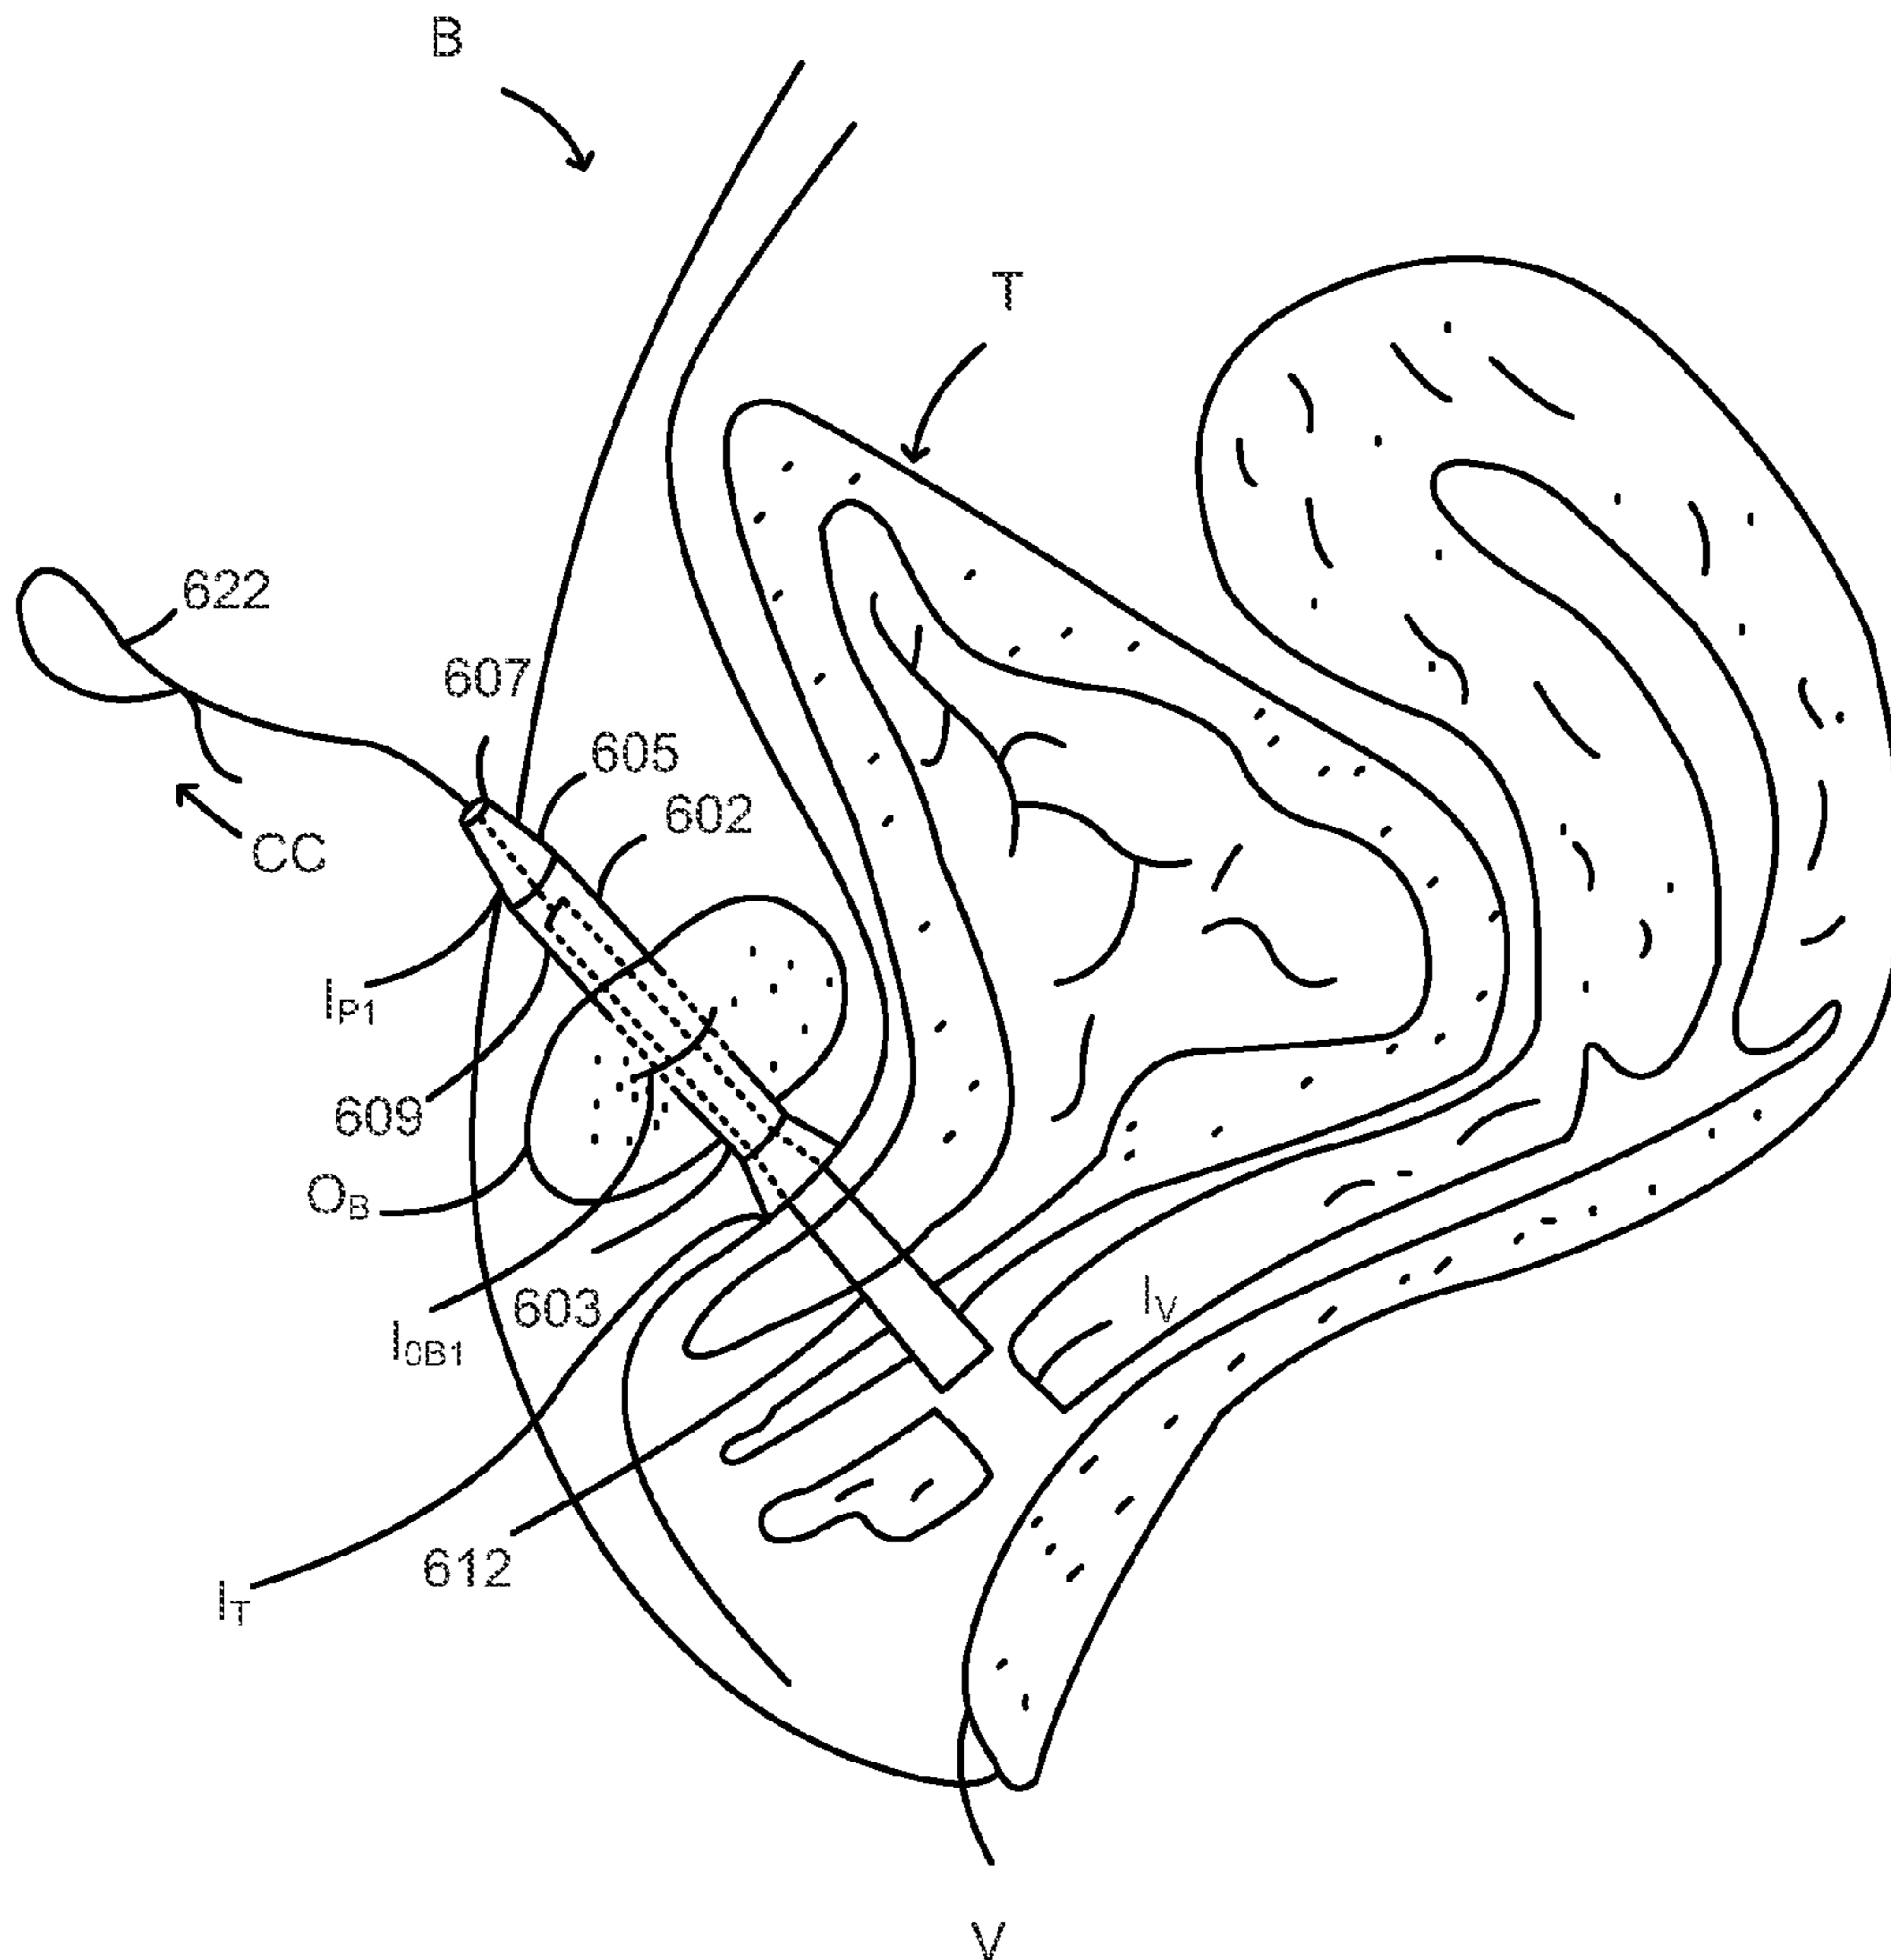


FIG. 14

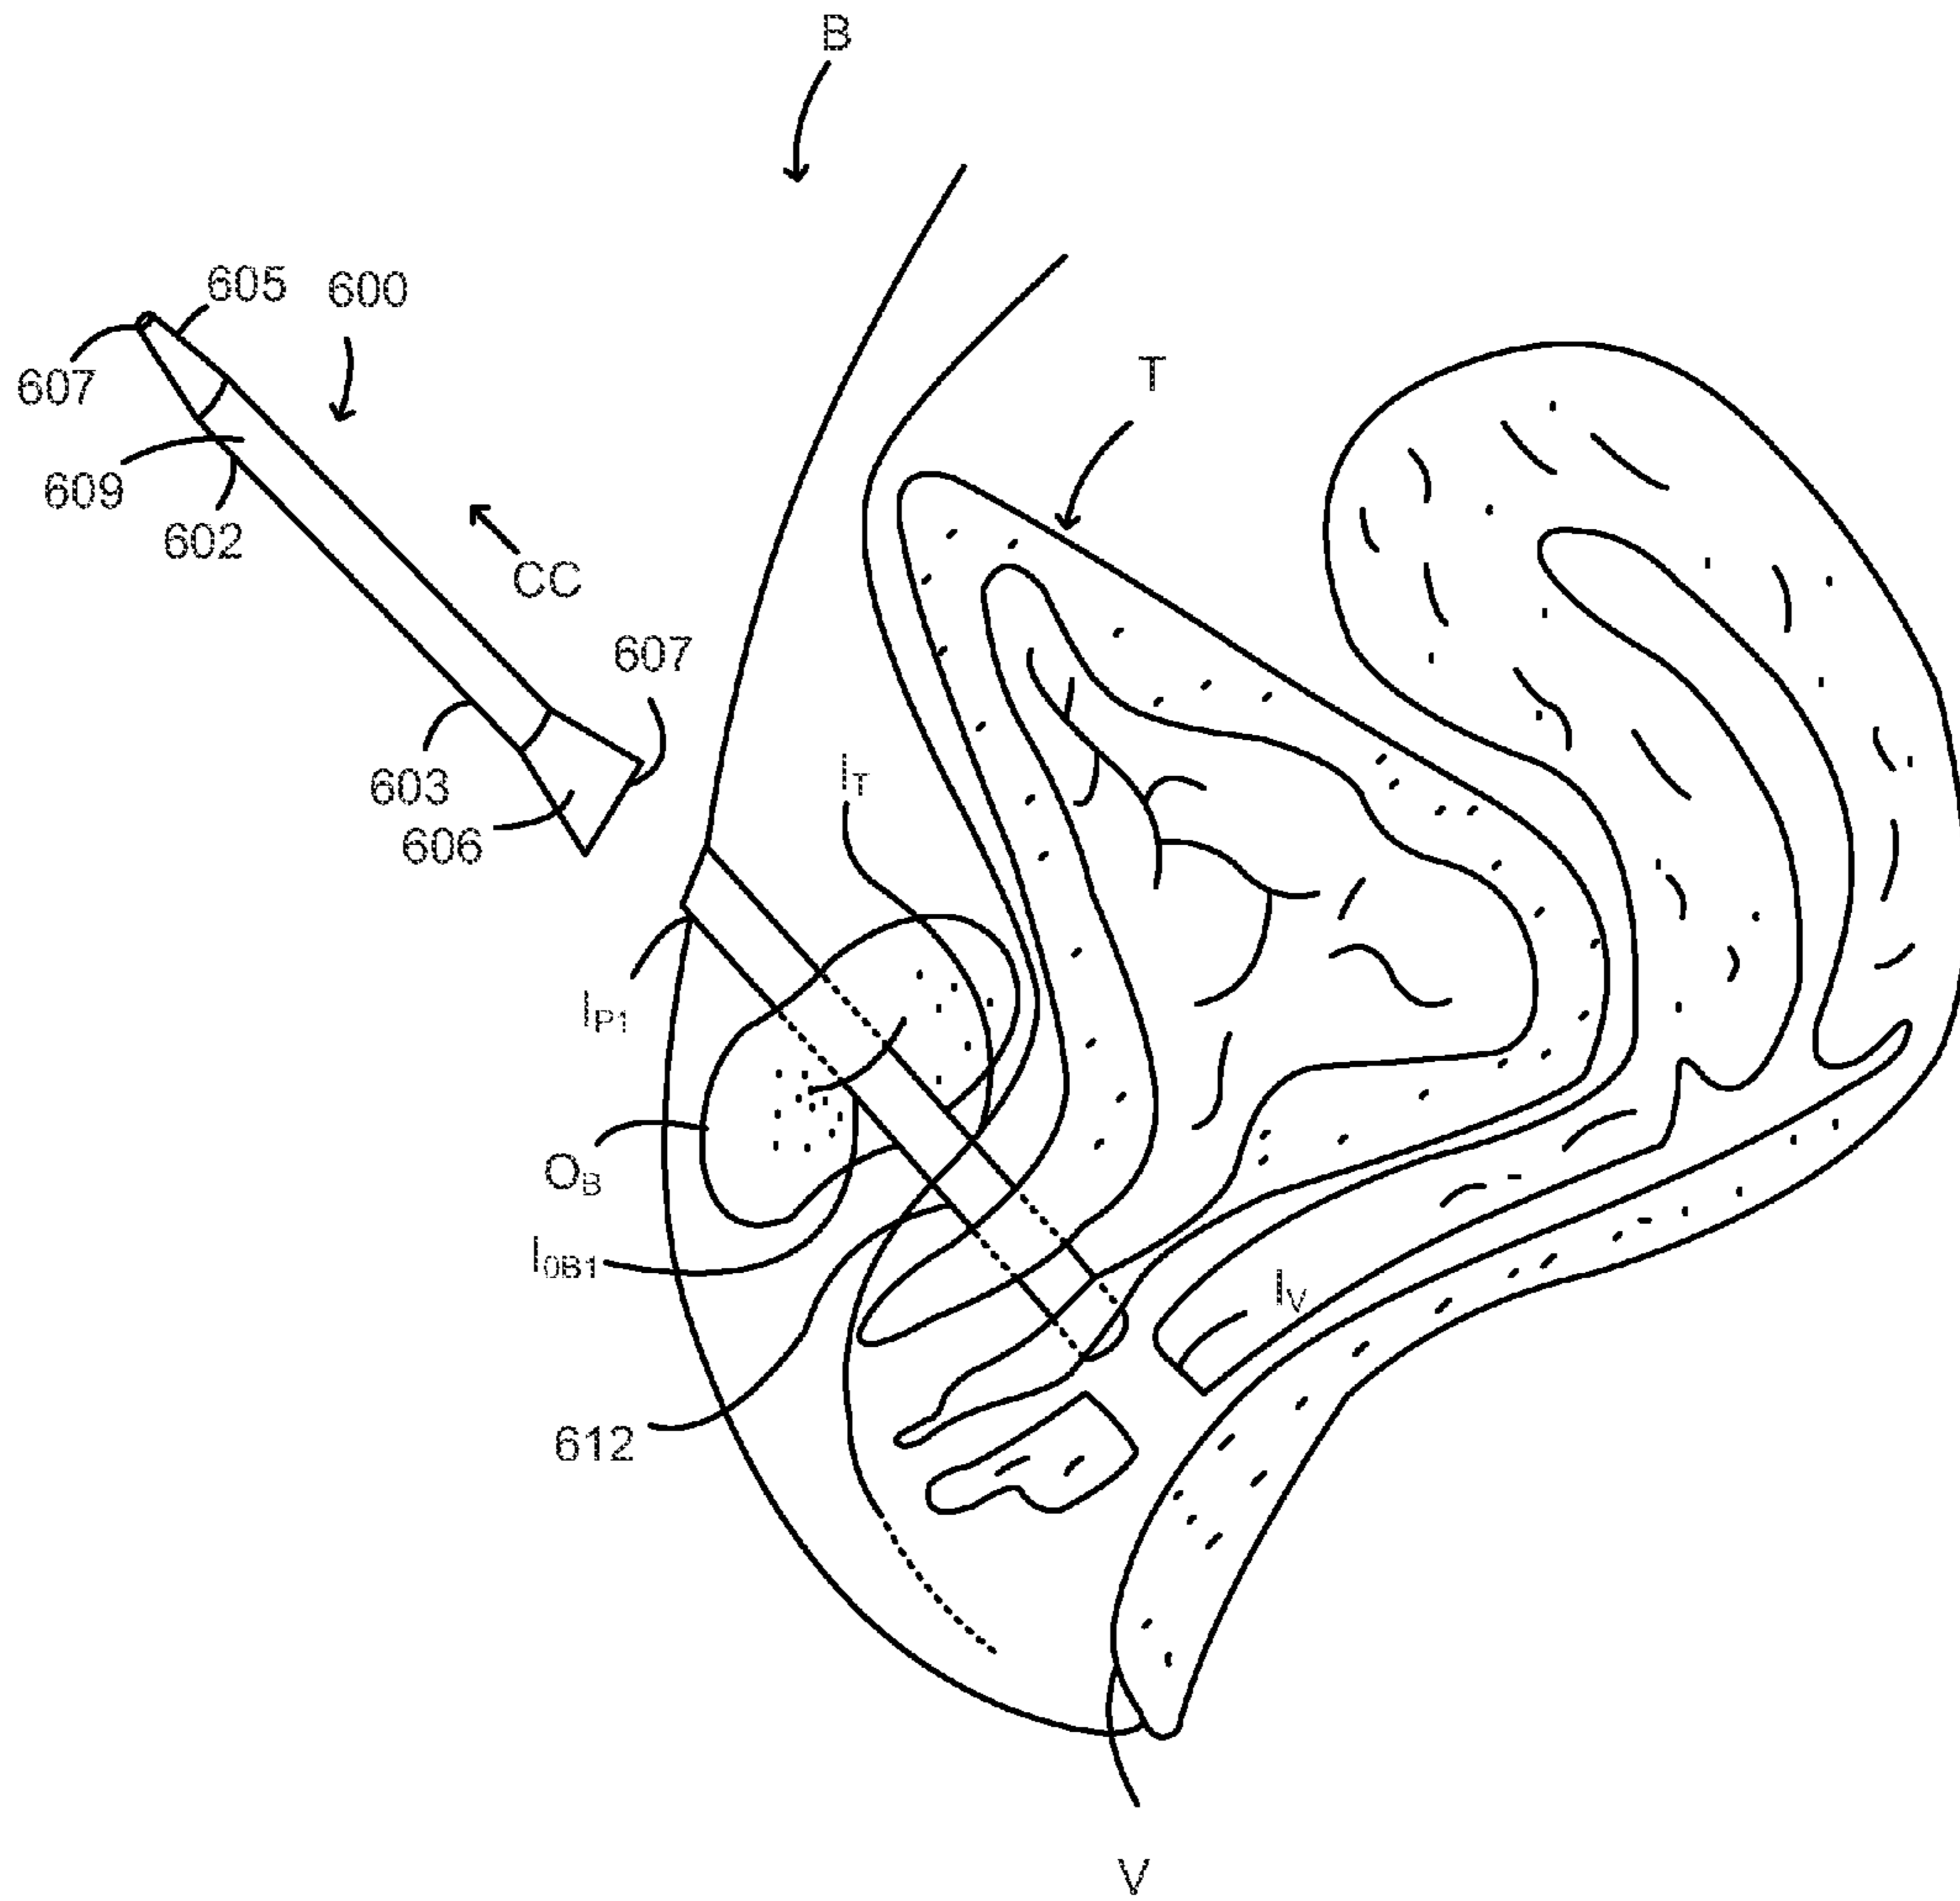


FIG. 15

1

**LESS TRAUMATIC METHOD OF DELIVERY  
OF MESH-BASED DEVICES INTO HUMAN  
BODY**

## RELATED APPLICATION

This application claims priority to and the benefit of U.S. Provisional Patent Application Ser. No. 61/289,898, filed on Dec. 23, 2009, entitled, "Less Traumatic Method of Delivery of Mesh-Based Devices Into Human Body," which is incorporated herein by reference in its entirety.

## BACKGROUND

The disclosed invention relates generally to medical devices and more particularly to implants and less traumatic methods for delivering implants within a pelvic region of a patient to treat various pelvic dysfunctions.

A variety of medical procedures are performed to treat various female pelvic dysfunctions, including procedures to treat urinary incontinence, and correcting various prolapse conditions such as uterine prolapse, cystoceles, rectoceles, and vaginal vault prolapse.

Women often experience vaginal prolapses due to age or other factors. For example, women may experience a cystocele, a rectocele and/or a hysterocele. A cystocele occurs when the bladder bulges into the vagina, and a rectocele occurs when the rectum bulges into the vagina. A hysterocele occurs when the uterus descends into the vagina. An enterocele (small bowel prolapse) can also occur, when the small bowel pushes through the upper wall of the vagina. It is relatively common for a hysterocele and cystocele or hysterocele and rectocele, or other combinations thereof to occur at the same time. It is also common for different types of prolapse to occur in relatively quick succession.

Treatment has included suturing procedures or the use of implants for support or suspension. A hysterocele is often treated with a hysterectomy followed by a vaginal vault suspension. Various devices and procedures are used to deliver and secure pelvic implants within a variety of different anatomical structures within a pelvic region. Implants can be delivered to a pelvic region through one or more vaginal incisions, and/or through exterior incisions in the patient.

Known methods of delivering or implanting implants, such as slings, within the body include the use of sleeves. In such known methods, a sleeve is disposed about the implant during insertion such that the sleeve and the implant are inserted within a bodily tissue. The sleeve, with the implant inside, is inserted through a bodily tissue. Once the implant is, for example, in a desired position within the bodily tissue, the sleeve can be removed from the body leaving the implant disposed within the bodily tissue. The sleeve protects the tissue from abrasion by the implant during delivery and adjustment, and protects the implant from over-stretching during delivery. The use of such known sleeves during implantation, however, can result in trauma to the bodily tissue through which the sleeve and implant have been inserted. More specifically, the sleeve adds bulk to the implant, and is typically stiffer than the implant, requiring larger incisions needed and/or holes created within the bodily tissue (for example, double the size). Undesirably large forces may also be required to pull the sleeved implant through a bodily tissue.

Thus, a need exists for a medical device that reduces trauma to the bodily tissue during insertion of an implant, i.e. by reducing the required size of the incision and/or the

2

hole through the tissue. Also, a need exists for a medical device that reduces the force required to move the device through the bodily tissue.

## SUMMARY

In some embodiments, a method includes extending a dilator into a body of a patient in a first direction such that a distal end portion of the dilator extends from the body. The dilator defines a lumen therethrough. At least a portion of the dilator is disposed within the body when the distal end portion extends from the body. At least a portion of an implant is passed through the lumen defined by the dilator. The dilator is removed from the body by moving the dilator in the first direction.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic illustration of a dilator according to an embodiment.

FIG. 2 is a schematic illustration of a delivery needle coupled to the dilator in FIG. 1 according to an embodiment.

FIG. 3 is a schematic illustration of a delivery needle coupled to the dilator in FIG. 1 according to another embodiment.

FIG. 4 is a flow chart of a method of inserting an implant into a body using the dilator in FIG. 1 according to an embodiment.

FIGS. 5-8 are schematic illustrations showing a method of inserting the implant into the body using the dilator in FIG. 1.

FIG. 9 is a schematic illustration of a dilator assembly according to an embodiment.

FIG. 10 is a flow chart of a method of inserting an implant into a body using the dilator assembly in FIG. 9 according to another embodiment.

FIGS. 11-15 are schematic illustrations showing a method of inserting the implant into the body using the dilator assembly in FIG. 9.

## DETAILED DESCRIPTION

The devices and methods described herein are generally directed to implants (e.g., slings for treatment of incontinence, such as by bladder neck suspension, posterior support implants, anterior support implants, and total pelvic floor repair implants) and the delivery and placement of such implants within a pelvic region of a patient using one or more dilators. An implant can be placed into the pelvic space of a patient and secured at one or more locations within the pelvic space to treat many different female pelvic floor dysfunctions.

The insertion device (i.e., the one or more dilators) is configured to place, deposit, or otherwise insert an implant (e.g., a sling) into one or more bodily tissues of a patient. The implant is configured to suspend or support a bodily tissue or organ when the implant is retained within the patient through tissue ingrowth and/or temporary suturing. For example, in one embodiment, the insertion device can place the implant under the bladder neck through the both obturator externus muscles and further through corresponding skin incisions for incontinence treatment.

As used in this specification, unless otherwise apparent from the context, the words "proximal" and "distal" refer to the direction closer to and further away from, respectively, an operator (e.g., surgeon, physician, nurse, technician, etc) who would use an insertion device during a procedure. For

example, the end of an insertion device first to contact the patient's body would be the distal end, while the opposite end of the insertion device (e.g., the end of the insertion device being operated by the operator) would be the proximal end of the insertion device. Similarly, the end of a 5 insertion device implanted the furthest within the patient's body would be the distal end, while the opposite end of the insertion device (e.g., the end of the insertion device that is inserted the least amount within the body or the end of the insertion device that is disposed outside of the body) would 10 be the proximal end.

FIG. 1 is a schematic illustration of a dilator **100** configured to be inserted within a body of a patient and to deliver an implant within the body. The dilator **100**, which can be, for example, a tube, includes a proximal end portion **103** and a distal end portion **102**. Additionally, the dilator **100** defines a distal opening **107**, a proximal opening **108** and a lumen (not identified) extending therethrough. The distal opening **107** is in fluid communication with the proximal opening **108** via the lumen. The lumen is configured to receive at least a portion of an implant (not illustrated) via the distal opening **107** and/or the proximal opening **108**, as described herein. The lumen is also configured to receive at least a portion of a delivery needle (not illustrated) via the distal opening **107** and/or the proximal opening **108**, as described herein.

The distal end portion **102** of the dilator **100** is configured to be inserted into a bodily tissue through an incision. Such a bodily tissue can be, for example, a vaginal tissue, an obturator membrane, a supra-pubic tissue, a retro-pubic tissue and/or the like. The distal end portion **102** of the dilator **100** may include a tapered tip **105**. The tapered tip **105** is configured to allow the dilator **100** to advance through the bodily tissue more easily. Said another way, the tapered tip **105** facilitates a smooth insertion of the dilator **100** into the bodily tissue. The tapered tip **105** can be tapered at any suitable angle (or rate) to reduce tissue resistance during insertion.

The proximal end portion **103** of the dilator **100** includes an enlarged portion **106**. The enlarged portion **106**, which may have, for example, a cone shape, is configured to operate as a funnel for the dilator **100**. For example, the enlarged portion **106** can receive, via the proximal opening **108**, a portion of an implant having a lateral dimension larger than a diameter of the lumen. The enlarged portion **106** can facilitate advancing the implant through the lumen by enabling the implant to gradually contract to a dimension sufficient to fit through the lumen without the exertion of undue force on the dilator **100** and/or the implant. In some instances, when the proximal end portion **103** of the dilator **100** is extended through a bodily tissue, the enlarged portion **106** provides a surgeon (or other doctor) a larger area with which to perform a procedure. The enlarged portion **106** can increase at any suitable angle (or rate). Although the enlarged portion **106** is illustrated and described above as having a cone shape (i.e., a circular funnel shape), in other embodiments, the enlarged portion **106** can have any suitable shape and/or size. For example, in some embodiments, the enlarged portion **106** can have a flat funnel shape. In some embodiments, however, the dilator **106** does not include an enlarged portion **106**.

In use, the dilator **100** is configured to engage a delivery needle (e.g., delivery needle **230** or **330** shown in FIGS. 2 and 3, respectively) prior to insertion into the body. The delivery needle is configured to either push or pull the dilator **100** through an incision and into the body, as described in more detail herein. In one example, the delivery needle can

push the dilator **100** through a vaginal incision. The delivery needle can further push the distal end portion **102** of the dilator **100** through the pelvic region of the body (including, for example, the retropubic space or the obturator foramina) and out of a skin incision, e.g. suprapubic or perineal. In such an example, the dilator **100** is positioned within the body such that the proximal end portion **103** is disposed flush with the first layer of tissue in which the implant is to be anchored and the distal end portion **102** is disposed through the skin incision, extending from the body.

Once the dilator **100** is positioned within the body, the delivery needle is disengaged from the dilator **100** and a portion of an implant can be advanced through the lumen of the dilator **100**. The implant can be, for example, a mesh sling or a mesh tape having a flat configuration or a rolled configuration. In some embodiments, a portion of the implant can be pushed through the dilator **100** in a distal direction via a pusher. In some embodiments, a portion of the implant can be coupled to a suture such that the suture is passed distally through the lumen and out of the distal opening **107** of the dilator **100**. The surgeon, for example, can then pull the suture and guide the implant into the lumen of the dilator **100** via the suture.

Once a suitable portion of the implant is disposed within the dilator **100**, the implant can be adjusted and/or tensioned. Since the length of the dilator **100** is sufficient to extend through body tissue from an entrance incision (e.g., in tissue in the pelvic region, accessed via a vaginal incision) to an exit incision (e.g. the supra-pubic incision), the implant can be inserted and positioned within the body within the dilator **100** without contacting any portion of the body other than the desired tissue or organ the implant is configured to support, as described in more detail herein. It should be understood that, although the procedure described above refers to only one dilator **100**, insertion of an implant, such as a sling, often involves the use of two dilators (see, for example, FIG. 9). For example, the dilator **100** can be used to implant a right portion of a sling and another dilator can be used to implant a left portion of the sling such that a body portion of the sling is disposed beneath and supports a bladder neck. In such an example, the dilator **100** extends through tissue in the retropubic region and a right supra-pubic incision, while the other dilator extends through tissue in the retropubic region and a left supra-pubic incision. Thus, an adjustment or tensioning of the sling can include adjusting the right portion of the sling relative to the left portion of the sling such that the body portion of the sling is properly tensioned to support the bladder neck.

The dilator **100** can be removed from the body after the implant is positioned within the body (albeit within the dilator **100**, which is within the body). The implant remains within the body and now contacts the bodily tissue between the supra-pubic incision site and the internal tissue incision. The vaginal incision can then be closed via suturing and/or the like. The portion of the implant extending from the external (e.g. supra-pubic) incision can be trimmed off, and the external incision can also be closed (with the portion of the implant disposed therein) via suturing and/or the like. In some embodiments, the dilator **100** can be removed from the body by moving the dilator **100** in the distal direction (i.e., the same direction as the insertion). In this manner, the proximal end portion **103** of the dilator **100** exits the body via the skin incision.

The dilator **100** can have any suitable shape and/or size. The dilator **100** can be constructed of any suitable, biocompatible material configured to be disposed within the body. For example, the dilator **100** can be constructed of a sub-

stantially rigid material, such as a stainless steel. In some embodiments, the dilator **100** can be constructed of a polymer. The dilator **100** can be formed, for example, by molding, extruding, casting, sintering, forging, machining, or other known methods of manufacturing, such medical devices.

The dilator **100** can have a substantially smooth and/or continuous outer surface to prevent or reduce friction produced between the dilator **100** and the bodily tissue when the dilator **100** contacts the bodily tissue during insertion. As friction between the dilator **100** and the bodily tissue decreases, the amount of force required to insert or move the dilator **100** through the bodily tissue decreases. Thus, the likelihood of damaging the bodily tissue during insertion also decreases.

In some embodiments, the distal end portion **102** of the dilator **100** can include an aperture (not illustrated in the embodiment of FIG. **11**, but illustrated, for example in the embodiment of FIG. **9**) through which a suture can extend. For example, as described above, the implant can be coupled to a suture such that the suture is passed through the dilator **100** and used to pull or guide the implant through the dilator **100**. In this embodiment, an end of the suture can be laced through the aperture and, for example, tied to the distal end portion **102** of the dilator **100** such that the suture is releasably coupled to the dilator **100** before insertion. In this manner, the dilator **100** is inserted within the body along with the suture. When the surgeon, for example, is ready to move the implant into the dilator **100**, the suture can be decoupled (untied), removed from the aperture and pulled in the same manner described above. In some embodiments, however, the suture can be fixedly coupled within the aperture and/or a distal end portion **102** of the dilator **100**.

FIG. **2** is schematic illustration of the dilator **100** coupled to a delivery needle **230** prior to insertion into a body. The delivery needle **230** is configured to push the dilator **100** through the body. The method of inserting the dilator **100** via the delivery needle **230**, as disclosed below, is herein referred to as the “push” method. The delivery needle **230** includes a handle **231** and a needle **232** with a tip **233**. The needle **232**, which has a slight curvature along its length, is coupled to the handle **231**.

When the delivery needle **230** is coupled to the dilator **100**, the needle **232** is disposed within the lumen defined by the dilator **100** such that the tip **233** of the needle **232** extends from the distal opening **107** of the dilator **100**. In some embodiments, the tip **233** and/or another portion of the needle **232** can form an interference fit with the dilator **100** when the needle **232** is disposed within the distal opening **107**. In this manner, the dilator **100** can be restricted from moving or uncoupling from the delivery needle **230** during insertion. On other embodiments, however, the needle **232** can be coupled to the dilator **100** in any other suitable manner.

In use, the delivery needle **230** is coupled to the dilator **100** in the manner described above, and inserted into the body, for example, via a vaginal incision. The delivery needle **230** can be operated, for example, by a surgeon. The delivery needle **230** is pushed through the body toward, for example, a supra-pubic incision, such that the dilator **100** is pushed through body tissue toward the supra-pubic incision. In some embodiments, the delivery needle **230** can be pushed through the body toward, for example, a retro-pubic incision, a perineum incision and/or the like. Additionally, in some embodiments, pushing the delivery needle **230**

through the body includes pushing the delivery needle **230** and a portion of the dilator **100** through an obturator membrane.

The advancement of the delivery needle **230** through the body is halted after the tip **233** of the delivery needle **230** reaches the supra-pubic incision (or other desired incision) and the distal end portion **102** of the dilator **100** extends from the body through the supra-pubic incision (or other desired incision), once the proximal opening **108** of the dilator is approximately flush with the body tissue into which the dilator **100** has been inserted. The delivery needle **230** can then be uncoupled from the dilator **100** and removed from the body. The delivery needle **230** is removed by moving (or pulling) the needle **232** in the opposite direction from which it was pushed through the body. In this manner, the delivery needle **230** is removed from the vaginal incision (i.e., the same incision through which it was inserted). The dilator **100** remains within the body.

FIG. **3** is a schematic illustration of the dilator **100** coupled to a delivery needle **330** during insertion into a body. The delivery needle **330** is configured to pull the dilator **100** through the body tissue. Thus, as will be described in more detail herein, the delivery needle **330** is configured to be inserted within the body before the dilator **100**. The method of inserting the dilator **100** via the delivery needle **330**, as disclosed below, is herein referred to as the “pull” method. The delivery needle **330** includes a handle **331** and a needle **332** with a tip **333**. The needle **332**, which has a C-shaped curvature, is coupled to the handle **331**. The needle **332** can have any suitable shape and/or size. For example, in some embodiments, the needle **332** can have the same shape and/or size as the needle **232** of the delivery needle **230** shown in FIG. **2**.

When the delivery needle **330** is coupled to the dilator **100**, the tip **333** of the needle **332** is disposed within, or adjacent to, the distal opening **107** defined by the dilator **100**. More specifically, as shown in FIG. **3**, the tip **333** of the needle **332** extends within the lumen of the dilator **100**. In some embodiments, the tip **333** and/or another portion of the needle **332** can form an interference fit with the dilator **100** when the needle **332** is disposed within the distal opening **107**. In this manner, the dilator **100** can be restricted from moving or uncoupling from the delivery needle **330** during insertion. In some embodiments, the tip **333** and/or another portion of the needle **332** can define a groove or recess configured to receive and/or couple to the distal end portion **102** of the dilator **100**.

In use, the delivery needle **330** is inserted into the body via an exit incision, such as, for example, a supra-pubic incision. The exit incision is the incision from which the distal end portion **102** of the dilator **100** will extend once placed, as discussed in more detail herein. In some embodiments, the exit incision can be, for example, a retro-pubic incision, a perineum incision and/or the like. The delivery needle **330**, which can be operated, for example, by a surgeon, is pushed through the body tissue toward an entry point adjacent the tissue or organ to be engaged by the implant. Once the tip **333** of the needle **332** passes through the entry point and enters a region of the pelvic area where it can be accessed (e.g. via a vaginal incision), the delivery needle **330** is coupled to the dilator **100** in the manner described above. The delivery needle **330**, with the dilator **100**, is then retracted or pulled back into the body in the opposite direction from which it was inserted.

The delivery needle **330** continues to retract through the body, pulling the dilator **100**, until the distal end portion **102** of the dilator **100** extends from the body through the

supra-pubic incision. In some embodiments, pulling the delivery needle **330** through the body includes pulling the delivery needle **330** and a portion of the dilator **100** through an obturator membrane and out through a perineal incision. The delivery needle **330** can then be uncoupled from the dilator **100** and removed from the body. In some embodiments, however, the delivery needle **330** is removed from or disposed outside of the body when the delivery needle **330** is uncoupled from the dilator **100**. In embodiments where a portion of the delivery needle **330** (e.g., the tip **333**) is disposed within the body when the delivery needle **330** is uncoupled from the dilator **100**, the delivery needle **330** can be removed by moving (or pulling) the remainder of the needle **332** from the body in the same direction along which it pulled the dilator **100** through the body. In this manner, the delivery needle **330** is removed from the supra-pubic incision the same incision through which it was inserted). The dilator **100** remains within the body.

The needles **232** and/or **332** can be constructed from any suitable material and can have any suitable shape and/or size, as discussed briefly above. Similarly, the handles **231** and/or **331** can be any suitable handle. The needles **232** and/or **332** can be constructed of any suitable material and can have any suitable shape and/or size.

In some embodiments, the needle (e.g., needle **232** and/or needle **233**) can include a coupling member (not illustrated) configured to couple the needle to the dilator **100**. The coupling member, which can be disposed on the distal end of the needle, is configured to be disposed within the lumen of the dilator **100** when the needle is coupled to the dilator **100**. In some embodiments, the coupling member can be portion of the needle having an increased diameter such that the needle is coupled to the dilator **100** via friction. Said another way, the dilator **100** and the needle can form an interference fit via the coupling member, when the coupling member is disposed within the lumen of the dilator **100**. In some such embodiments, the coupling member can be remotely controlled such that the diameter of that portion of the needle can increase and/or decrease on command. The coupling member can be actuated, for example, by pulling a wire on a handle (e.g., handle **231** and/or **331**) of the needle, by pushing a button disposed on the handle, by squeezing a portion of the handle, and/or the like.

In some embodiments, the coupling member can include female threads configured to receive male threads disposed on the distal end portion **102** of the dilator **100**. In this manner, the needle (e.g., needle **232** and/or needle **233**) and the dilator **100** are releasably and threadedly coupled together.

FIG. **4** is a flow chart of a method **450** of inserting an implant **510** into a body B of a patient. The method illustrated in FIG. **4** is discussed with references FIGS. **5-8**, which are schematic illustrations of the implant **510** being inserted into the body B via dilators **100** and **500**. The term “implant” will be referred to herein as a “sling,” unless otherwise specified. It should be understood, however, that the implant **510** can be any suitable implant including, but not limited to, a sling. For example, the implant **510** can be a mesh tape having a flat configuration or a rolled configuration. The method **450** includes extending a dilator through a body tissue of a patient in a first direction such that a distal end portion of the dilator extends from the body tissue, **451**. Referring to FIGS. **5** and **6**, the dilator **100** extends through the body B of the patient in a distal direction AA such that the distal end portion **102** of the dilator **100** extends from the body B. Similarly, the dilator **500** extends through the body B of the patient in a distal direction BB such that a distal end

portion **502** of the dilator **500** extends from the body B. The dilator **500** has substantially the same structure and operation as dilator **100** and thus, will not be described in detail herein. Also, it should be understood that, during the procedures described herein, the dilator **500** performs the same steps or operations that dilator **100** performs. Therefore, when the dilator **100** is described as or referred to in performing a particular step or operation, it should be understood that dilator **500** is also involved in or performing that particular step or operation, unless otherwise specified.

The dilator **100** is inserted into the body B of the patient via a vaginal incision,  $I_V$  (shown in FIG. **6**). The dilator **500** is also inserted into the body B of the patient via the vaginal incision  $I_V$ . In this manner, there is only a single incision in the vaginal wall V through which both dilators **100** and **500** are inserted to access the tissue through which they will extend to the exterior of the body B, i.e. through incisions in the skin of body B. The incision  $I_V$  can be made at any suitable location along the vaginal wall V depending on the intended implantation site of the sling **510** within the pelvic region. For example, the vaginal incision  $I_V$  is shown in FIG. **6** as being located in the anterior vaginal wall V proximate the mid-urethra (i.e., the intended implantation location/site).

The distal end portion **102** of the dilator **100** extends from the body B of the patient via a first supra-pubic incision  $I_{S1}$ . Similarly, the distal end portion **502** of the dilator **500** extends from the body B of the patient via a second suprapubic incision  $I_{S2}$ . The first supra-pubic incision  $I_{S1}$  is located toward the right side of the body B and the second supra-pubic incision  $I_{S2}$  is located toward the left side of the body B relative to the perspective of the patient. In some embodiments, however, the supra-pubic incisions  $I_{S1}$  and  $I_{S2}$  can be made at any location in the supra-pubic region of the body B. In some embodiments, the location of the supra-pubic incisions  $I_{S1}$  and/or  $I_{S2}$  can depend, for example, on the intended implantation site of the sling **510** within the pelvic region.

The dilator **100** can be inserted into the body B using one of the methods described above with reference to FIGS. **2** and **3**. More particularly, the dilator **100** can be pushed into the body B (through body tissue) using, for example, the delivery needle **230** (i.e., the “push” method). Or, the dilator **100** can be pulled into the body B using, for example, the delivery needle **330** the “pull” method), in most instances, however, the “push” method is regularly used for procedures involving supra-pubic incisions. As such, the dilator **100** is inserted into the body B by being pushed through the vaginal incision  $I_V$  and further through the pelvic region (including, the tissue in the supra-pubic space), in distal direction AA, until the distal end portion **102** of the dilator **100** extends from the first supra-pubic incision  $I_{S1}$ . In some embodiments, the dilator **100** can be inserted into the body B in a manner different from the dilator **500**. For example, the dilator **100** can be inserted into the body B via the “push” method, and the dilator **500** can be inserted into the body B via the “pull” method. Regardless of the method used to insert the dilators **100** or **500**, the dilator **100** is moved through the body B in direction AA during insertion and dilator **500** is moved through the body B in direction BB during insertion.

When the dilator **100** is extended through the body B, as shown in FIGS. **5** and **6**, the proximal end portion **103** of the dilator **100** is disposed within at least the first layer of tissue  $T_1$  (via a first tissue layer incision  $I_T$ ) in which the sling **510** is to be anchored and a proximal-most end (not identified) of the dilator **100** is flush with that first layer of tissue  $T_1$ . In

some embodiments, however, the proximal-most end of the dilator **100** can be flush with the vaginal wall **V** (i.e., the vaginal tissue). The placement of the proximal-most end of the dilator **100** can facilitate a more accurate placement of the sling **510** at the desired implantation site within the body **B**. For example, the ability to tension and/or adjust the sling **510** with respect to the urethra (or another desired implantation site) may be restricted in instances where the proximal-most end(s) of the dilators **100** and/or **500** extend beyond the first layer of tissue  $T_1$ . In instances where the proximal-most end(s) of the dilators **100** and/or **500** are recessed within that first layer of tissue  $T_1$ , the tissue surrounding the first tissue layer incision  $I_T$  can close up around the dilator **100**. In some embodiments, however, the proximal-most end of the dilator **100** can be recessed within the first layer of tissue  $T_1$  or can extend into the vagina through the vaginal incision **h**.

As shown in FIG. **5**, a first suture **522** is disposed within the lumen defined by the dilator **100**. The first suture **522** has a first portion (not identified), which extends from the distal opening **107** of the dilator **100**, and a second portion (not identified), which is coupled to a first arm **512** of the sling **510**. Similarly, a second suture **523** is disposed within the lumen defined by the dilator **500**. The second suture **523** has a first portion (not identified), which extends through the distal opening **507** of the dilator **500**, and a second portion (not identified), which is coupled to a second arm **513** of the sling **510**. As discussed in more detail herein, the sutures **522** and **523** are configured to facilitate the placement of the sling **510** within the body **B**. During this phase of the implantation procedure, however, the sling **510** may remain outside of the body **B**.

Returning to the flow chart shown in FIG. **4**, at least a portion of an implant can be passed through the lumen defined by the dilator, **452**. As shown in FIG. **7**, the first arm **512** of the sling **510** is passed or moved in distal direction **AA** through the lumen defined by the dilator **100**. More specifically, the first portion of the first suture **522** is moved in distal direction **AA** (i.e., away from the body **B** and/or the dilator **100**) such that the first arm **512** of the sling **510** is moved in the distal direction **AA**. The first suture **522** can continue to be moved or pulled in the distal direction **AA** until the first arm **512** of the sling **510** is in the desired position within the lumen defined by the dilator **100**. The desired position of the first arm **512** of the sling **510** within the lumen can, for example, correspond to the desired location of the sling **510** within the body **B** after implantation. Such a desired position can be achieved by, for example, adjusting and/or tensioning the first arm **512** of the sling **510** within the lumen relative to the second arm **513**. The first suture **522** is, therefore, configured to guide the first arm **512** of the sling **510** into the lumen defined by the dilator **100** and to facilitate its placement within the lumen.

As shown in FIG. **7**, the dilator **100** is configured to act a barrier between the first arm **512** of the sling **510** and the body **B** (including the body tissue through which the dilator is passed) when the first arm **512** is disposed within the lumen of the dilator **100**. Said another way, the dilator **100** substantially prevents the first arm **512** of the sling **510** from contacting body tissue (other than the organ it is intended to support) when the first arm **512** is disposed within the lumen of the dilator **100**. The first arm **512** of the sling **510** has a length sufficient to extend through body tissue from the vaginal incision  $I_V$  or the desired implantation site, to the first supra-pubic incision  $I_{S1}$ . The length of the first arm **512** of the sling **510**, however, is shorter than the length of the dilator **100**. As a result, the first arm **512** of the sling **510**

remains within the lumen of the dilator **100** while at least the first portion of the suture **522** extends through the distal opening **107** of the dilator **100** and outside of the body **B**. In some embodiments, however, the first arm **512** of the sling **510** can have any suitable length. For example, in some embodiments, the length of the first arm **512** of the sling **510** can be greater than the length of the dilator **100** such that a portion of the first arm **512** can extend through the distal opening **107** of dilator and/or outside of the body **B**.

Returning to the flow chart shown in FIG. **4**, the dilator is removed from the body tissue by moving the dilator in the first direction, **453**. As shown in FIG. **8**, the dilator **100** is removed from the body **B** by moving the dilator **100** in the distal direction **AA**. In this manner, the dilator **100** is inserted into the body **B** and removed from the body **B** in the same direction. Thus, the dilator **100** enters the body **B** via the vaginal incision  $I_V$  and exits the body **B** via the first supra-pubic incision  $I_{S1}$ .

As shown in FIG. **8**, the sling **510** remains within the body **B** after the dilator **100** is removed from the body **B**. Thus, the sling **510** is in contact with the body tissue between the first supra-pubic incision  $I_{S1}$  and the first layer tissue incision  $I_T$  after the dilator **100** is removed from the body **B**. In some embodiments, the sling **510** can be configured to promote tissue ingrowth in the surrounding bodily tissue (e.g., the tissue between the first supra-pubic incision and the first layer tissue incision  $I_T$  and/or the tissue of the organ) after the dilator **100** is removed and the sling **510** is placed in contact with the tissue of body **B**.

The sling **510** maintains a substantially constant position within the body **B** when the dilator **100** is removed.

Once the dilator **100** is removed from the body **B**, the sutures **522** and/or **523** can be trimmed off or otherwise removed from the respective arms **512** and/or **513** of the sling **510**. The sling **510** itself can also be trimmed after the dilator **100** is removed from the body **B**. Additionally, the vaginal incision  $I_V$ , the first tissue layer incision  $I_T$  (or any other internal incisions), and/or each of the supra-pubic incisions  $I_{S1}$  and  $I_{S2}$  can be closed via any suitable manner.

Although the sling **510** is illustrated and described above as being coupled to sutures **522** and **523**, in other embodiments, the sling **510** is not coupled to sutures. In such embodiments, the first arm **512** of the sling **510** can be passed through the lumen defined by the dilator **100** via, a pusher or like device. Similarly, the second arm **513** of the sling **510** can be passed through the lumen defined by the dilator **500** via a pusher or like device. In some embodiments, the sling **510** is attached to only one of the sutures **522** or **523**.

FIG. **9** is a schematic illustration of a dilator assembly, which includes dilators **600** and **700** coupled to an implant **610**. The dilators **600** and **700** are configured to be inserted within a body of a patient and to deliver the implant **610** within the body. The term "implant" will be referred to herein as a "sling" in the same manner discussed above with reference to implant **510** (i.e., sling **510**). The dilator **600** includes a proximal end portion **603** having an enlarged portion **606**, and a distal end portion **602** having a tapered tip **605**. Additionally, the dilator **600** defines a distal opening **607**, a proximal opening **608**, an aperture **609** and a lumen (not identified) extending therethrough. The dilator **600** has substantially the same structure and operation as dilator **100**, but includes an aperture **609** in the distal end portion **602** of the dilator **600**. Thus, the proximal end portion **603**, the distal end portion **602**, the enlarged portion **606**, and the tapered tip **605** have substantially the same structure and operation as the proximal end portion **103**, the distal end



portion 102, the enlarged portion 106, and the tapered tip 105 of the dilator 100, and are, therefore, not described in detail herein unless otherwise specified. Additionally, the distal opening 607, the proximal opening 608, and the lumen 5 have substantially the same structure and operation as the distal opening 107, the proximal opening 108, and the lumen defined by the dilator 100, and are, therefore, not described in detail herein unless otherwise specified. Furthermore, the dilator 700 has substantially the same structure and operation as dilator 600 and thus, will not be described in detail 10 herein unless otherwise specified.

The aperture 609 is located in the distal end portion 602 of the dilator 600. The aperture 609 is configured to receive a portion of a first suture 622, as described in more detail 15 herein. The aperture 609 can have any suitable shape and/or size. For example, although the aperture 609 is illustrated in FIG. 9 as having a substantially circular shape, in other embodiments, the aperture 609 can have, for example, an oval shape, a square shape, a star shape and/or the like. Additionally, the aperture 609 can be formed by any suitable 20 process, such as, for example, molding, drilling, casting, or the like.

The sling 610 is operatively coupled to the dilators 600 and 700 via sutures 622 and 623, respectively. The sling 610 is configured to be implanted within the body to support a 25 desired tissue or organ within the body. The sling 610, which is illustrated in FIG. 9 as a flat mesh tape, includes a first arm 612 and a second arm 613. The first arm 612 is coupled to a second portion (not identified) of the first suture 622, and the second arm 613 is coupled to a second portion (not 30 identified) of the second suture 623. As will be described in more detail herein, the first arm 612 is configured to be implanted within the body via the dilator 600 and the second arm 613 is configured to be implanted within the body via the dilator 700. The arms 612 and 613 are configured to be 35 received within the lumens of the dilators 600 and 700, respectively.

As shown in FIG. 9, the first suture 622 is disposed within at least a portion of the lumen defined by the dilator 600 40 when the second portion of the first suture 622 is coupled to the first arm 612 of the sling 610. The first suture 622 includes a first portion (not identified) that extends through the aperture 609 (i.e., from the inside-out) and is coupled to the distal end portion 602 of the dilator 600 via the aperture 609. In some embodiments, the first portion of the first 45 suture 622 can include a knot to prevent the first portion from receding back through the aperture 609, which thereby couples the first suture 622 to the dilator 600. The first portion of the first suture 622, however, can include any suitable anchor to prevent the first portion from receding 50 back through the aperture 609. For example, in some embodiments, the first portion of the first suture 622 can be fixedly coupled within the aperture 609 via an adhesive.

The first portion of the first suture 622 can be coupled to the distal end portion 602 of the dilator 600 via the aperture 55 609 in any suitable manner. For example, in some embodiments, the first portion of the first suture 622 can be pulled through the distal opening 607 of the dilator 600 and then laced through the aperture 609 from the outside-in. A knot can be formed at the first portion of the first suture 622 to 60 prevent the first suture 622 from receding back through the aperture 609. In some embodiments, a portion of the exposed first suture 622 can further be formed into a loop (shown, for example, in FIGS. 11 and 12). The surgeon, for example, can exert a force on the first suture 622 via the loop 65 such that the knot (or other anchor) is forced through the aperture 609, thereby uncoupling the first suture 622 from

the dilator 600. The loop can then be used to pull or move the first arm 612 of the sling 610 into the lumen of the dilator 600, as described herein.

In some embodiments, a kit can include the dilators 600 and 700 and the implant 610. In some such embodiments, the kit can be pre-assembled such that the implant 610 is coupled to the dilators 600 and 700 via sutures 622 and 623, respectively. The implant 610 can be coupled to the dilators 600 and/or 700 in any manner described herein. In some 10 embodiments, the sling 610 can be pre-formed into a roll and included in the kit. In this manner, the sling 610 can be inserted into the body in its pre-formed configuration and can, for example, unroll into its original configuration at some time during or after the implantation procedure.

FIG. 10 is a flow chart of a method 860 of inserting an implant 610 into a body B of a patient. The method illustrated in FIG. 10 is discussed with references FIGS. 11-15, which are schematic illustrations of the implant 610 being inserted into the body B via the dilator assembly shown in 15 FIG. 9. The term “implant” will be referred to herein as a “sling,” as discussed above. The method 860 includes extending a dilator through a body tissue of a patient such that a distal end portion of the dilator extends from the body tissue, 861. Referring to FIGS. 11 and 12, the dilator 600 25 extends through the body B (including internal body tissue) of the patient such that the distal end portion 602 of the dilator 600 extends from the body B. Similarly, the dilator 700 extends through the body B of the patient such that a distal end portion 702 of the dilator 700 extends from the 30 body B. It should be understood that, during the procedures described herein, the dilator 700 performs the same steps or operations that dilator 600 performs. Therefore, when the dilator 600 is described as or referred to in performing a particular step or operation, it should be understood that dilator 700 is also involved in or performing that particular 35 step or operation, unless otherwise specified.

The dilator 600 is inserted into the body B via a vaginal incision,  $I_V$  (shown in FIG. 12). The dilator 700 is also inserted into the body B via the vaginal incision  $I_V$ . In this 40 manner, there is only a single incision in the vaginal wall  $I_V$  through which both dilators 600 and 700 extend. In some embodiments, however, the dilators 600 and/or 700 are inserted into the body B via separate vaginal incisions. The incision  $I_V$  can be made at any location along the vaginal wall V depending on the intended implantation site of the 45 sling 610 within the pelvic region, as described above. When the dilator 600 is extended through the body B, as shown in FIG. 12, the proximal end portion 603 of the dilator 600 is disposed within at least the first layer of tissue  $T_1$  (via, a first tissue layer incision  $I_T$ ) in which the sling 510 is to be anchored and a proximal-most end (not identified) of the dilator 600 is flush with that first layer of tissue  $T_1$  as 50 described above.

As shown in FIG. 12, the dilator 600 extends through an obturator membrane  $O_B$  within the body B when the distal 55 end portion 602 of the dilator 600 extends through the body 13. More particularly, the dilator 600 extends through a first obturator incision  $I_{OB1}$  when the distal end portion 602 of the dilator 600 extends from a first perineum incision  $I_{P1}$ . Similarly, the dilator 700 extends through the opposing 60 obturator membrane (not illustrated) via a second obturator incision (not illustrated) when the distal end portion 702 of the dilator 700 ends from the body B via a second perineum incision  $I_{P2}$ . The first perineum incision  $I_{P1}$  and the obturator membrane  $O_B$  are located toward the right side of the body B, and the second perineum incision  $I_{P2}$  and opposing 65 obturator membrane are located toward the left side of the

body B relative to the perspective of the patient. In some embodiments, however, the perineum incisions  $I_{P1}$  and  $I_{P2}$  can be made at any location in the perineum region of the body B. Similarly, the obturator incisions (e.g., the first obturator incision  $I_{OB1}$ ) can be made at any location along the obturator membranes the obturator membrane  $O_B$ ) The location of the perineum incisions  $I_{P1}$  and/or  $I_{P2}$  can depend, for example, on the intended implantation site of the sling **610** within the pelvic region.

The dilator **600** can be inserted into the body B using one of the methods described above with reference to FIGS. **2** and **3**. More particularly, the dilator **600** can be pushed through the body B using, for example, the delivery needle **230** (i.e., the “push” method). Or, the dilator **600** can be pulled through the body B using, for example, the delivery needle **330** (i.e., the “pull” method). In most instances, however, the “pull” method is regularly used for procedures involving perineum and/or obturator incisions. As such, the delivery needle (e.g., delivery needle **330**) is inserted and moved within the body B along a path that includes the first perineum incision  $I_{P1}$ , the first obturator incision  $I_{OB1}$ , the first tissue layer incision  $I_T$  (and any other internal body tissue incisions) and the vaginal incision  $I_V$ . Once the delivery needle reaches the vaginal incision  $I_V$ , the distal end portion **602** of the dilator **600** can be coupled to the delivery needle, in the manner described above, and inserted into the body B. The dilator **600** is inserted into the body B by being pulled in distal direction CC through the vaginal incision  $I_V$ , through the first tissue layer incision  $I_T$ , through the obturator incision  $I_{OB1}$ , and further through the first perineum incision  $I_{P1}$  until the distal end portion **602** of the dilator **600** extends through the first perineum incision  $I_{P1}$ . In some embodiments, the dilator **700** can be inserted into the body B in a manner different from the dilator **600**, as discussed above.

The dilators **600** and **700** are inserted into the body B in a similar configuration to that shown in FIG. **9**. Similar to the configuration shown in FIG. **9**, the sling **610** is operatively coupled to the dilators **600** and **700** via sutures **622** and **623** when the dilators **600** and **700** are inserted within the body B. The sutures **622** and **623** shown in FIGS. **11** and **12**, however, are in a looped configuration. More specifically, with respect to dilator **600**, the first portion of the first suture **622** extends through the lumen and out from the distal opening **607**, then loops around the outside of the dilator **600** and through the aperture **609**. The first portion of the first suture **622** disposed through the aperture **609** is then securely fastened to the dilator **600**, for example, via a knot, as described above. A loop (not identified) is then formed with the portion of the first suture **622** disposed outside of the dilator **600**. During this phase of the implantation procedure, the sling **610** remains outside of the body B.

Returning to the flow chart shown in FIG. **10**, the first portion of the suture is uncoupled from the distal end portion of the dilator, **862**. As shown in FIG. **13**, the first portion of the first suture **622** is uncoupled from the distal end portion **602** of the dilator **600** when the first suture **622** is moved in direction CC. A surgeon, for example, can pull the first suture **622** (e.g., via the loop) such that the force exerted on the first suture **622** in the distal direction CC forces the knot through the aperture **609** and, thereby uncouples the first suture **622** from the distal end portion **602** of the dilator **600**. In some embodiments, however, the first portion of the first suture **622** is uncoupled from distal end portion **602** of the dilator **600** in any suitable manner, such as, for example, via severing.

Returning to the flow chart shown in FIG. **10**, at least a portion of an implant is passed through the lumen defined by the dilator by pulling on the first portion of the suture, **863**. As shown in FIG. **14**, the first arm **612** of the sling **610** is passed or moved through the lumen defined by the dilator **600** by pulling the first portion of the first suture **622** in distal direction CC. For example, once the first suture **622** is uncoupled from the distal end portion **602** of the dilator **600**, the surgeon, for example, can continue to pull the first suture **622** (e.g., via the loop) in the distal direction CC until the first arm **612** of the sling **610** is pulled into the lumen of the dilator **600**. In some embodiments, the acts of pulling the first portion of the first suture **622** to uncouple it from the dilator **600** and to pull the sling **610** into the dilator **600** is performed in a continuous motion. In some embodiments, the first suture **622** can continue to be pulled until the first arm **612** of the sling **610** is in the desired position within the lumen defined by the dilator **600**. As described above, the desired position of the first arm **612** of the sling **610** within the lumen can, for example, correspond to the desired location of the sling **610** within the body B after implantation. Such a desired position can be achieved by, for example, adjusting and/or tensioning the first arm **612** of the sling **610** within the lumen relative to the second arm **613**.

As shown in FIG. **14** and described above, when the first arm **612** is disposed within the lumen of the dilator **600**, the dilator **600** is configured to act a barrier between the first arm **612** of the sling **610**, the obturator membrane  $O_B$  and the body B (including any bodily tissue other than the tissue or organ it is intended to support). The first arm **612** of the sling **610** has a length sufficient to extend through body tissue from the vaginal incision  $I_V$  or the desired implantation site, to the first perineum incision  $I_{P1}$ . The length of the first arm **612** of the sling **610**, however, is shorter than the length of the dilator **600**. As a result, the first arm **612** of the sling **610** remains within the lumen of the dilator **600** while at least the first portion of the first suture **622** extends through the distal opening **607** of the dilator **600** and outside of the body B, as described above. In some embodiments, however, the first arm **612** of the sling **610** can have any suitable length, as described above. For example, in some embodiments, the length of the first arm **612** is only sufficient to extend from the vaginal incision  $I_V$  or the desired implantation site, to the first obturator incision  $I_{OB1}$ .

Returning to the flow chart shown in FIG. **10**, the dilator is removed from the body tissue through a skin incision, **864**. As shown in FIG. **15**, the dilator **600** is removed from the body B through the first perineum incision  $I_{P1}$ . In this manner, the dilator **600** is inserted into the body B and removed from the body B in the same direction (i.e., distal direction CC). Thus, the dilator **600** enters the body B via the vaginal incision  $I_V$  and exits the body B via the first perineum incision  $I_{P1}$ . In some embodiments, however, the dilator **600** can be removed from the body B through the vaginal incision  $I_V$ . In this manner, the dilator **600** is inserted and removed from the same incision.

As shown in FIG. **15**, the sling **610** remains within the body B after the dilator **600** is removed from the body B, as described above. Thus, the sling **610** is in contact with the body tissue between the first layer tissue incision  $I_T$  and the first perineum incision  $I_{P1}$  (including the obturator membrane  $O_B$ ) after the dilator **600** is removed from the body B. In some embodiments, the sling **610** can be configured to promote tissue ingrowth in the surrounding bodily tissue, including the obturator membrane  $O_B$ , after the dilator **600** is removed and the sling **610** is placed in contact with the body B.

Once the dilators **600** and **700** are removed from the body B, the sutures **622** and/or **623** can be trimmed off or otherwise removed from the respective arms **612** and/or **613** of the sling **610**. The sling **610** itself can also be trimmed off after the dilators **600** and **700** are removed from the body B. Additionally, the vaginal incision  $I_V$ , the first layer tissue incision  $I_T$ , the obturator incision  $I_{OB1}$  and/or each of the perineum incisions  $I_{P1}$  and  $I_{P2}$  can be closed via any suitable manner.

Although the sling **610** is illustrated and described above as being coupled to sutures **622** and **623**, in other embodiments, the sling **610** is not coupled to sutures. In such embodiments, the first arm **612** of the sling **610** can be passed through the lumen defined by the dilator **600** via a pusher or like device. Similarly, the second arm **613** of the sling **610** can be passed through the lumen defined by the dilator **600** via a pusher or like device. In some embodiments, the sling **610** is attached to only one of the sutures **622** or **623**.

While various embodiments of the invention have been described above, it should be understood that they have been presented by way of example only, and not limitation. Thus, the breadth and scope of the invention should not be limited by any of the above-described embodiments, but should be defined only in accordance with the following claims and their equivalents. While the invention has been particularly shown and described with reference to specific embodiments thereof, it will be understood that various changes in form and details may be made.

Although the dilators illustrated and described above were used to delivery or implant an implant into a pelvic region via a specific approach, in other embodiments, the dilator(s) can be used to deliver or implant an implant into a pelvic region using a variety of different approaches, including for example, a transvaginal approach, a retropubic approach, a supra pubic approach, or a transobturator approach.

Although the dilators are illustrated and described above as being positioned within the body such that the proximal end portion of the dilators are disposed within the vaginal area and the distal end portion of the dilators are disposed adjacent the outer surface of the body, in other embodiments, a dilator is positioned within the body in the opposite configuration. For example, the dilator can be positioned within the body such that the distal end portion of the dilator is disposed within the vaginal area and the proximal end portion of the dilator is disposed adjacent the outer surface of the body. In some such embodiments, a suture coupled to an implant, or the implant itself, is pulled into the lumen of the dilator via the distal opening. In this manner, the suture and/or the implant moves or passes through the lumen of the dilator in the opposite direction to that described above (i.e., from the distal end portion of the lumen to the proximal end portion of the lumen). The suture and/or the implant can be moved through the lumen by any of the means described above. For example, in some embodiments, the suture and/or the implant is coupled to a delivery needle (e.g., delivery needle **230** or **330**) and pulled through the lumen.

Although the dilators and procedures are illustrated and described above with reference to a female pelvic region, it should be understood that the same dilators and/or procedures can be used in the male pelvic region without substantial modification. For example, where the female pelvic region is accessed via a vaginal incision in the aforementioned procedures, the male pelvic region can be accessed via right and left perineum incisions. In some embodiments,

the female pelvic region can be accessed via perineum incisions rather than a vaginal incision in the aforementioned procedures.

The implant(s) described herein can be formed with a variety of different materials, such as biocompatible plastics and/or metals. In some embodiments, the implant is formed at least in part with a mesh material to promote tissue in-growth. An implant can also be formed fully or in part with biological or natural materials or combinations of biological and synthetic materials. An implant can be formed at least in part with, for example, the Advantage® Mesh by Boston Scientific Corporation. Alternatively, the implant can be formed with Polyform® Synthetic Mesh material by Boston Scientific Corporation.

The implant(s) can have a variety of different configurations and/or different sizes (e.g. lengths, widths), depending on the intended use for the particular implant and the intended implantation site for the implant within the pelvic region.

The previous description of the embodiments is provided to enable any person skilled in the art to make or use the invention. While the invention has been particularly shown and described with reference to embodiments thereof, it will be understood by those skilled in art that various changes in form and details may be made. For example, a dilator can include various combinations and sub-combinations of the various embodiments described herein.

In some embodiments, a method includes extending a dilator into a body tissue of a patient in a first direction such that a distal end portion of the dilator extends from the body of the patient. The dilator defines a lumen therethrough. At least a portion of the dilator is disposed within the body tissue when the distal end portion extends from the body. At least a portion of an implant is passed through the lumen defined by the dilator. The dilator is removed from the body tissue by moving the dilator in the first direction.

In some embodiments, the dilator can be extended by pushing the distal end portion of the dilator through the body tissue.

In some embodiments, the dilator can be extended by pulling the distal end portion of the dilator through the body tissue.

In some embodiments, the dilator can be extended into a portion of the body tissue in a pelvic region of the patient.

In some embodiments, the dilator can be extended such that a proximal end of the dilator is aligned with a surface of the body tissue. In this manner, the proximal end is flush with the surface.

In some embodiments, the distal end portion of the dilator can be configured to contact a portion of a delivery needle when the dilator is being extended into the body tissue.

In some embodiments, the dilator can be extended into the body tissue via a first incision, and is removed from the body via a second incision.

In some embodiments, the portion of the implant can be passed through the lumen by pushing the portion of the implant through the lumen in the first direction.

In some embodiments, the portion of the implant can be passed through the lumen by pulling the portion of the implant through the lumen in the first direction.

In some embodiments, the portion of the implant can be passed through the lumen in a second direction opposite the first direction.

In some embodiments, the first direction can be a distal direction.

In some embodiments, a proximal end portion of the dilator can include an enlarged portion, which is in fluid

communication with the lumen. In some such embodiments, the enlarged portion can be configured to facilitate the passing of the portion of the implant through the lumen.

In some embodiments, the implant can be configured to be used to treat male incontinence.

In some embodiments, a method includes extending a dilator into body tissue of a patient such that a distal end portion of the dilator extends from the body of the patient. The distal end portion of the dilator is coupled to a first portion of a suture such that the first portion of the suture is disposed outside of the body when the distal end portion of the dilator extends from the body. The suture has a second portion coupled to an implant. The dilator defines a lumen therethrough. The first portion of the suture is uncoupled from the distal end portion of the dilator and at least a portion of the implant is passed through the lumen defined by the dilator by pulling on the first portion of the suture. The dilator is removed from the body tissue through a skin incision.

In some embodiments, the method can also include coupling the first portion of the suture to the distal end portion of the dilator. In some such embodiments, the distal end portion of the dilator can define an aperture through which the first portion of the suture is disposed.

In some embodiments, after the dilator is removed from the body tissue, the method can also include, trimming the portion of the implant that extends from the bodily tissue such that the suture is detached from the implant.

In some embodiments, the dilator can be extended into a body tissue in a pelvic region of the patient.

In some embodiments, the dilator can be extended into the body tissue in a first direction, and can be removed from the body tissue in a direction substantially the same as the first direction.

In some embodiments, the dilator can be extended into the body tissue in a first direction, and can be removed from the body tissue in a second direction substantially opposite the first direction.

In some embodiments, the dilator can be extended into the body tissue and through a portion of an obturator.

In some embodiments, the distal end portion of the dilator can be configured to contact a portion of a delivery needle when the dilator is being extended into the body tissue.

In some embodiments, the suture can be uncoupled by pulling on a loop formed by the first portion of the suture such that the first portion of the suture uncouples from the distal end portion of the dilator.

In some embodiments, the incision can be one of a supra-pelvic incision, a retro-pubic incision, or a perineum incision.

In some embodiments, the implant can be configured to be used to treat male incontinence.

In some embodiments, the implant can be a mesh implant. What is claimed is:

**1.** A method, comprising:

inserting a needle of a delivery needle into a lumen of a first dilator, wherein, when the needle is inserted into the lumen of the first dilator, a tip of the needle extends outside the lumen from a first opening of the first dilator;

extending the first dilator into a body of a patient via a vaginal incision in a direction until a distal end portion of the first dilator extends from a first supra-pubic incision, the first dilator defining the first opening disposed proximate the distal end portion and a second opening disposed proximate to a proximal end portion of the first dilator, the lumen of the first dilator extend-

ing from the first opening to the second opening, at least a portion of the first dilator being disposed within the body when the distal end portion extends from the body, wherein a first suture extends through at least a portion of the lumen of the first dilator, the first suture having a first end portion coupled to an implant;

passing, after the extending, a first portion of the implant through the vaginal incision and then into the lumen defined by the first dilator by pulling on a second end portion of the first suture;

removing the first dilator from the body via the first supra-pubic incision by moving the first dilator in a direction that is the same as the direction used to extend the first dilator into the body of the patient while the portion of the first portion of the implant slides out of the lumen defined by the first dilator and remains in the body, wherein the removing includes removing the needle of the delivery needle from the body of the patient via the vaginal incision and removing the first dilator from the body of the patient via the first supra-pubic incision;

extending a second dilator into the body of the patient via the vaginal incision until a distal end portion of the second dilator extends from a second supra-pubic incision,

wherein a second suture extends through at least a portion of the lumen of the second dilator, the second suture having a first end portion coupled to a second portion of the implant, the first dilator and the second dilator extending into the body of the patient via the same vaginal incision;

passing, after the extending, the second portion of the implant through the vaginal incision and then into the lumen defined by the second dilator.

**2.** The method of claim 1, wherein the extending includes pushing the distal end portion of the first dilator through the body.

**3.** The method of claim 1, wherein the extending includes pulling the distal end portion of the first dilator through the body.

**4.** The method of claim 1, wherein the extending includes extending the first dilator into a portion of the body in a pelvic region of the patient.

**5.** The method of claim 1, wherein the extending includes aligning the proximal end portion of the first dilator with a surface of the body such that the proximal end portion is flush with the surface.

**6.** The method of claim 1, wherein, during the extending, the distal end portion of the first dilator is configured to contact a portion of the delivery needle.

**7.** The method of claim 1, wherein the passing includes pushing the portion of the implant through the lumen of the first dilator in a direction that is the same as the direction used to extend the first dilator into the body of the patient.

**8.** The method of claim 1, wherein the passing includes pulling the portion of the implant through the lumen of the first dilator in a direction that is the same as the direction used to extend the first dilator into the body of the patient.

**9.** The method of claim 1, wherein the direction used to extend the first dilator into the body of the patient is a distal direction.

**10.** The method of claim 1, wherein the proximal end portion of the first dilator includes an enlarged portion in fluid communication with the lumen of the first dilator, the enlarged portion configured to facilitate the passing.

19

11. A method, comprising:  
 inserting a needle of a delivery needle into a lumen of a dilator, the delivery needle also including a handle extending the needle, the dilator defining a first opening at a distal end portion of the dilator and a second opening at a proximal end portion of the dilator such that the lumen extends from the first opening to the second opening, wherein, when the needle is inserted into the lumen of the dilator, a tip of the needle extends outside the lumen from the first opening of the dilator;  
 pushing the needle and the dilator into a body of a patient via a vaginal incision until the distal end portion of the dilator extends from a supra-pubic incision, the distal end portion of the dilator being coupled to a first portion of a suture such that the first portion of the suture is disposed within the body when the distal end portion of the dilator extends from the body via the supra-pubic incision, the suture having a second portion coupled to an end portion of an implant, the distal end portion of the dilator defining an aperture proximate to the first opening, the suture extending through the aperture;  
 uncoupling the first portion of the suture from the distal end portion of the dilator;  
 passing, after the extending, at least a portion of the implant through the vaginal incision and then into the lumen defined by the dilator by pulling on the first portion of the suture and moving the suture through the aperture;

20

removing the needle of the delivery needle from the body of the patient through the vaginal incision; and  
 removing the dilator from the body of the patient through the supra-pubic incision.

12. The method of claim 11, further comprising:  
 coupling the first portion of the suture to the distal end portion of the dilator, the distal end portion of the dilator defining the aperture through which the first portion of the suture is disposed.

13. The method of claim 11, further comprising:  
 after the removing, trimming the portion of the implant extending through the bodily tissue such that the suture is detached from the implant.

14. The method of claim 11, wherein the pushing includes pushing the dilator into a portion of the body in a pelvic region of the patient.

15. The method of claim 11, wherein the pushing includes pushing the needle and the dilator into the body in a direction towards the supra-pubic incision, and the removing includes removing the dilator from the body via the supra-pubic incision by moving the dilator in a direction substantially the same as the direction used to push the dilator into the body.

16. The method of claim 11, wherein the pushing includes pushing the dilator into the body and through a portion of an obturator.

\* \* \* \* \*