

US009561028B1

(12) **United States Patent**
Fan

(10) **Patent No.:** **US 9,561,028 B1**
(45) **Date of Patent:** **Feb. 7, 2017**

(54) **AUTOMATIC LAPAROSCOPIC KNOT TYING INSTRUMENT**

(71) Applicant: **Peter Fan**, Saddle River, NJ (US)

(72) Inventor: **Peter Fan**, Saddle River, NJ (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **14/973,858**

(22) Filed: **Dec. 18, 2015**

(51) **Int. Cl.**

A61B 17/04 (2006.01)

A61B 17/02 (2006.01)

A61B 17/06 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 17/0469** (2013.01); **A61B 17/0482** (2013.01); **A61B 17/0483** (2013.01); **A61B 17/0485** (2013.01); **A61B 2017/0474** (2013.01); **A61B 2017/0496** (2013.01)

(58) **Field of Classification Search**

CPC **A61B 17/0469**; **A61B 17/0482**; **A61B 17/0483**; **A61B 17/0485**; **A61B 2017/0474**; **A61B 2017/0496**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,320,629	A *	6/1994	Noda	A61B 17/0469
					606/113
5,501,690	A *	3/1996	Measamer	A61B 17/0469
					606/144
5,520,702	A *	5/1996	Sauer	A61B 17/0469
					29/751

(Continued)



Primary Examiner — Matthew F Desanto

(57) **ABSTRACT**

In laparoscopic surgery, tying of knots is not easy, as it involves the use of long handled graspers and the necessity to pass one end of the suture ligature around the opposite half of the suture, with release and re-grab of the passing end of the suture. The present invention avoids the “passing with the release and re-grab”, and makes the tying easier, faster and automatic. It conforms to the general size and shape of a standard laparoscopic instrument. The handle is pistol shaped with two control triggers, one for grasping and the other for rotating. The sheath is elongated and tubular, containing two control rods. The tip is bullet shaped, containing three operating mechanisms, one for grasping the leading end of a suture, a second for trapping the opposite half of the same suture, a third for rotating the grasped end of the suture 360 degrees around the trapped portion, thus forming a knot.

The trapping mechanism uses an axle with a hollow center and an open-ended side slot. The other members of the rotating and trapping mechanisms have these same features, which allow the suture to enter and exit the hollow center. Grasping is performed by a miniature grasper, which has no handle or shaft, with its entire body contained within a part that rotates, called the rotator. Rotation is generated by a slider-crank mechanism which converts linear motion to rotary motion, and avoids the dead centers with a patented L-shaped connecting rod and deflecting pillars (U.S. Pat. No. 9,194,468). The rotation is then transmitted through two modified spur gears to the rotator, and hence also to the miniature grasper. The rotator represents a short sagittal segment removed from the tip, modified to rotate and to contain the miniature grasper, and then replaced in position. To enable the grasper to rotate, there is an intentional discontinuity in its controlling rod, but control from the handle is maintained by the interposition of a semi-open ball and socket joint in the rod.

2 Claims, 24 Drawing Sheets

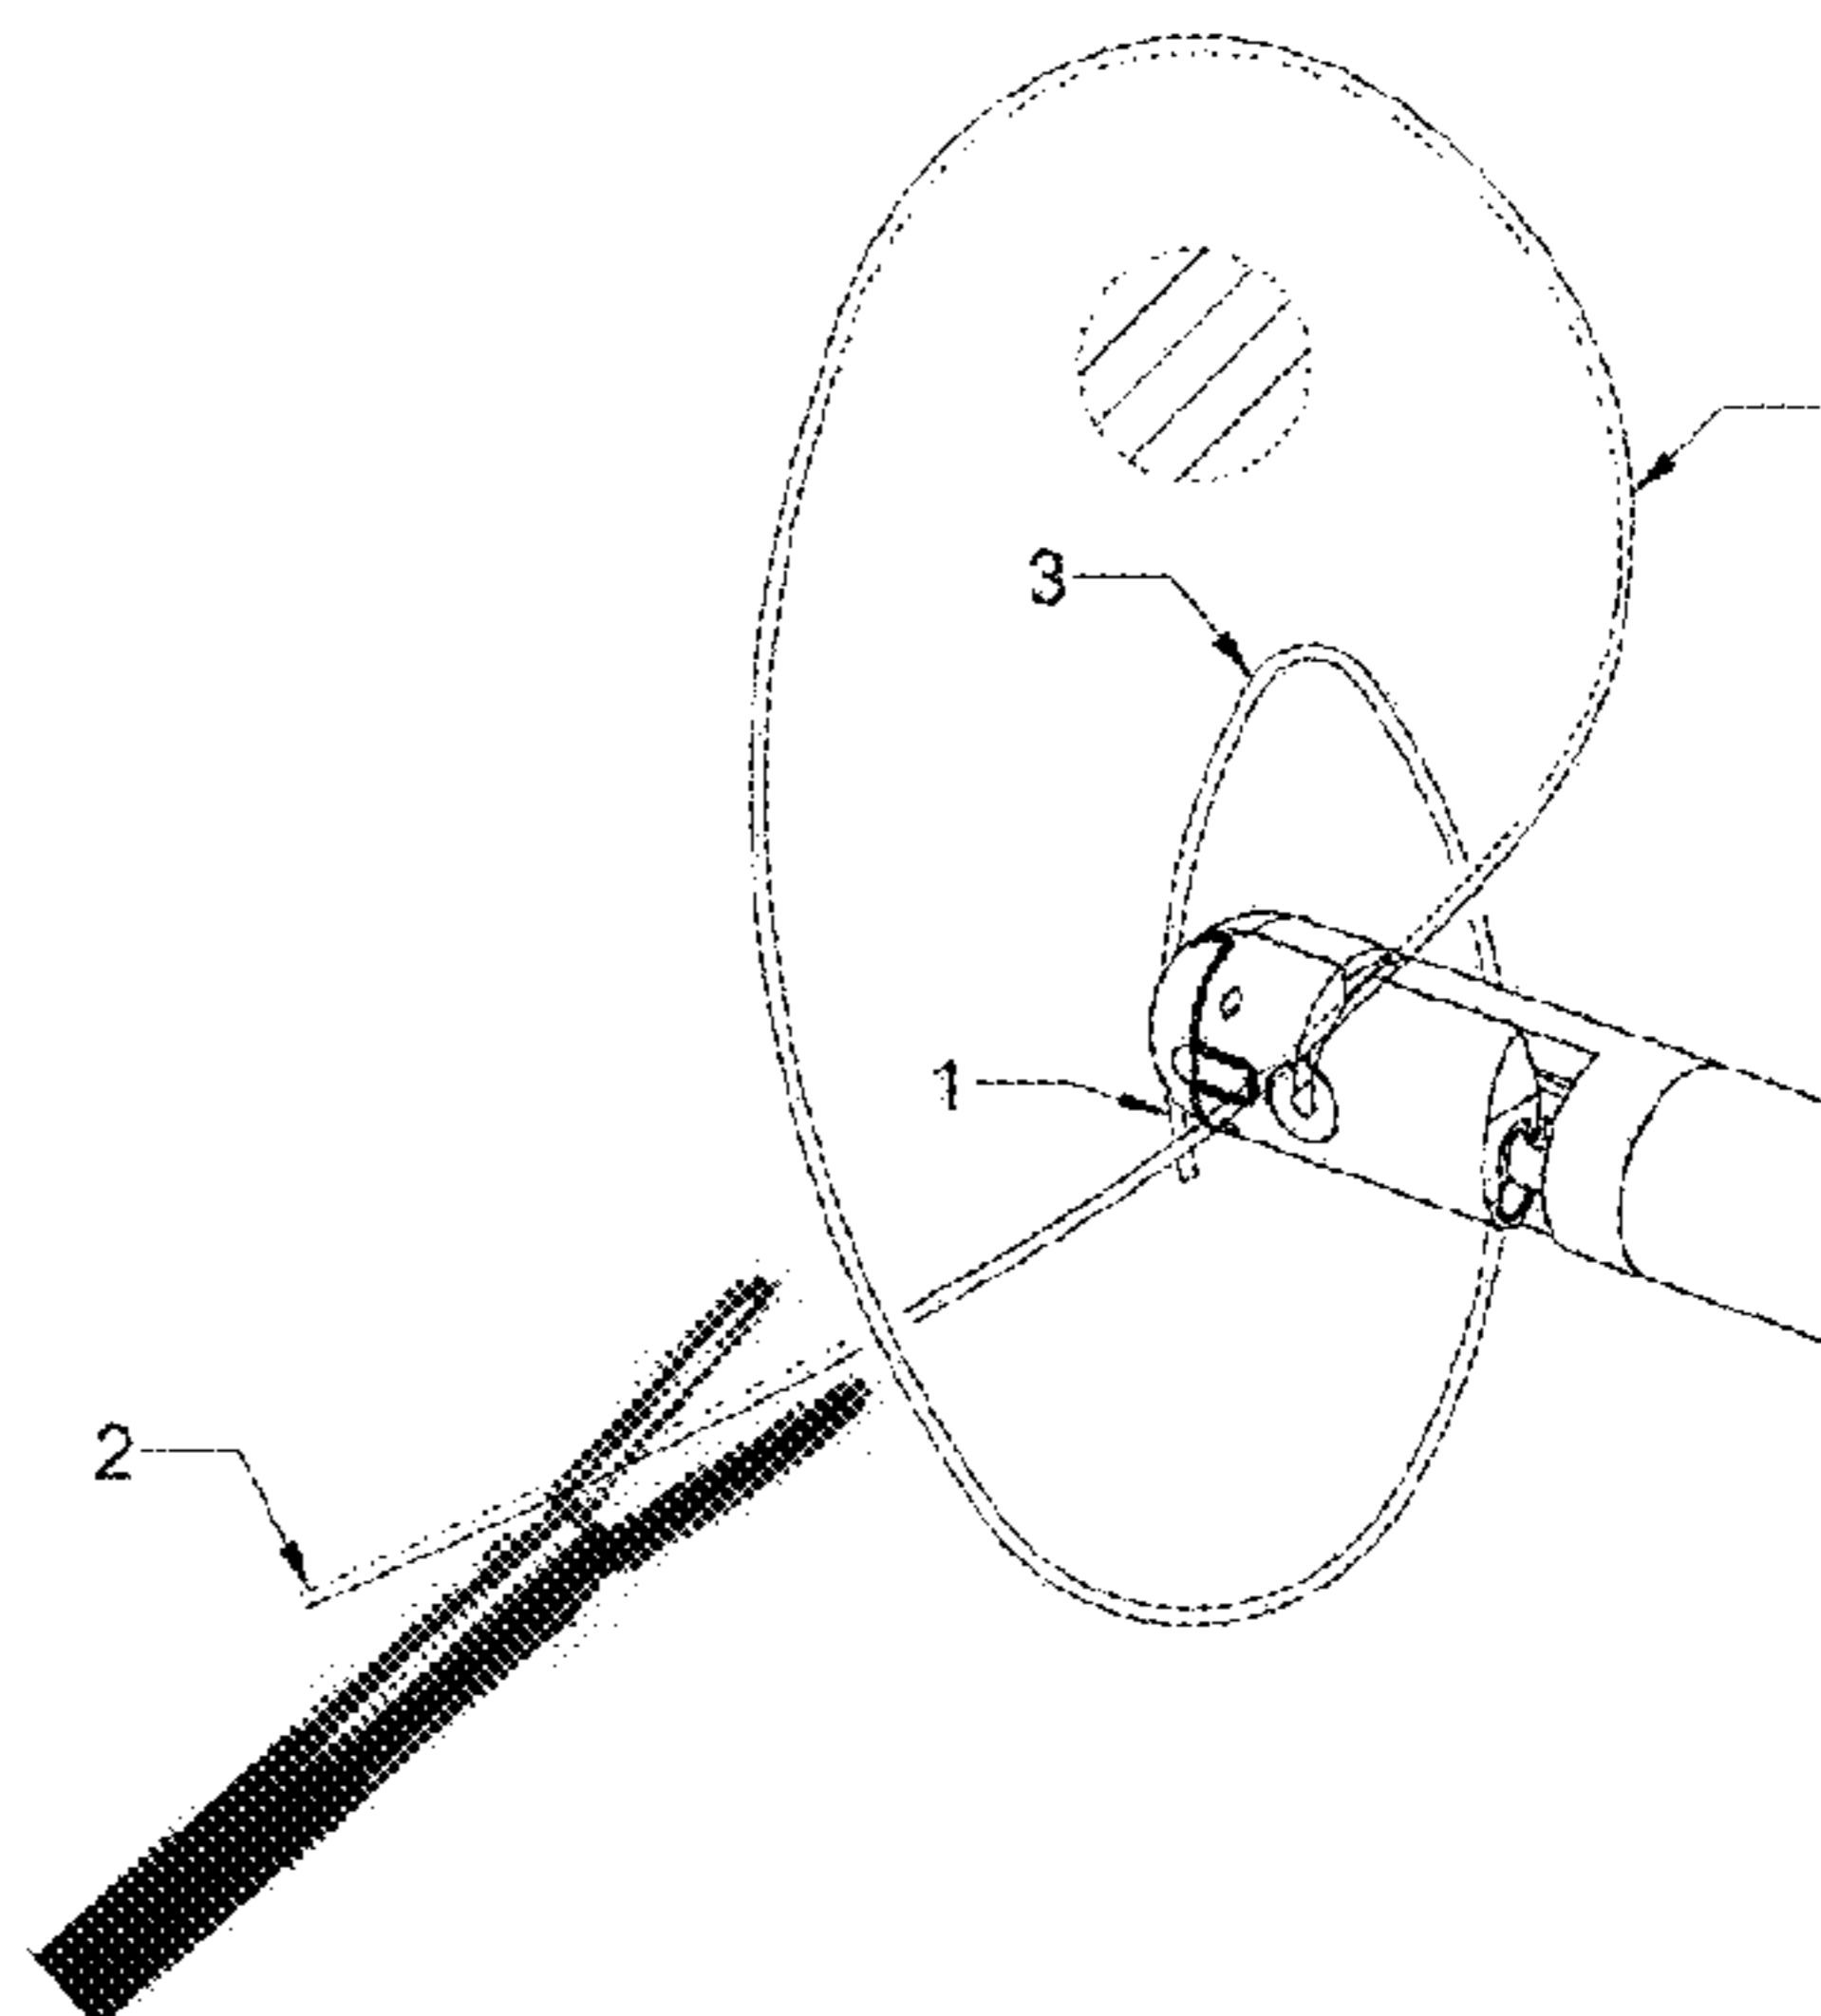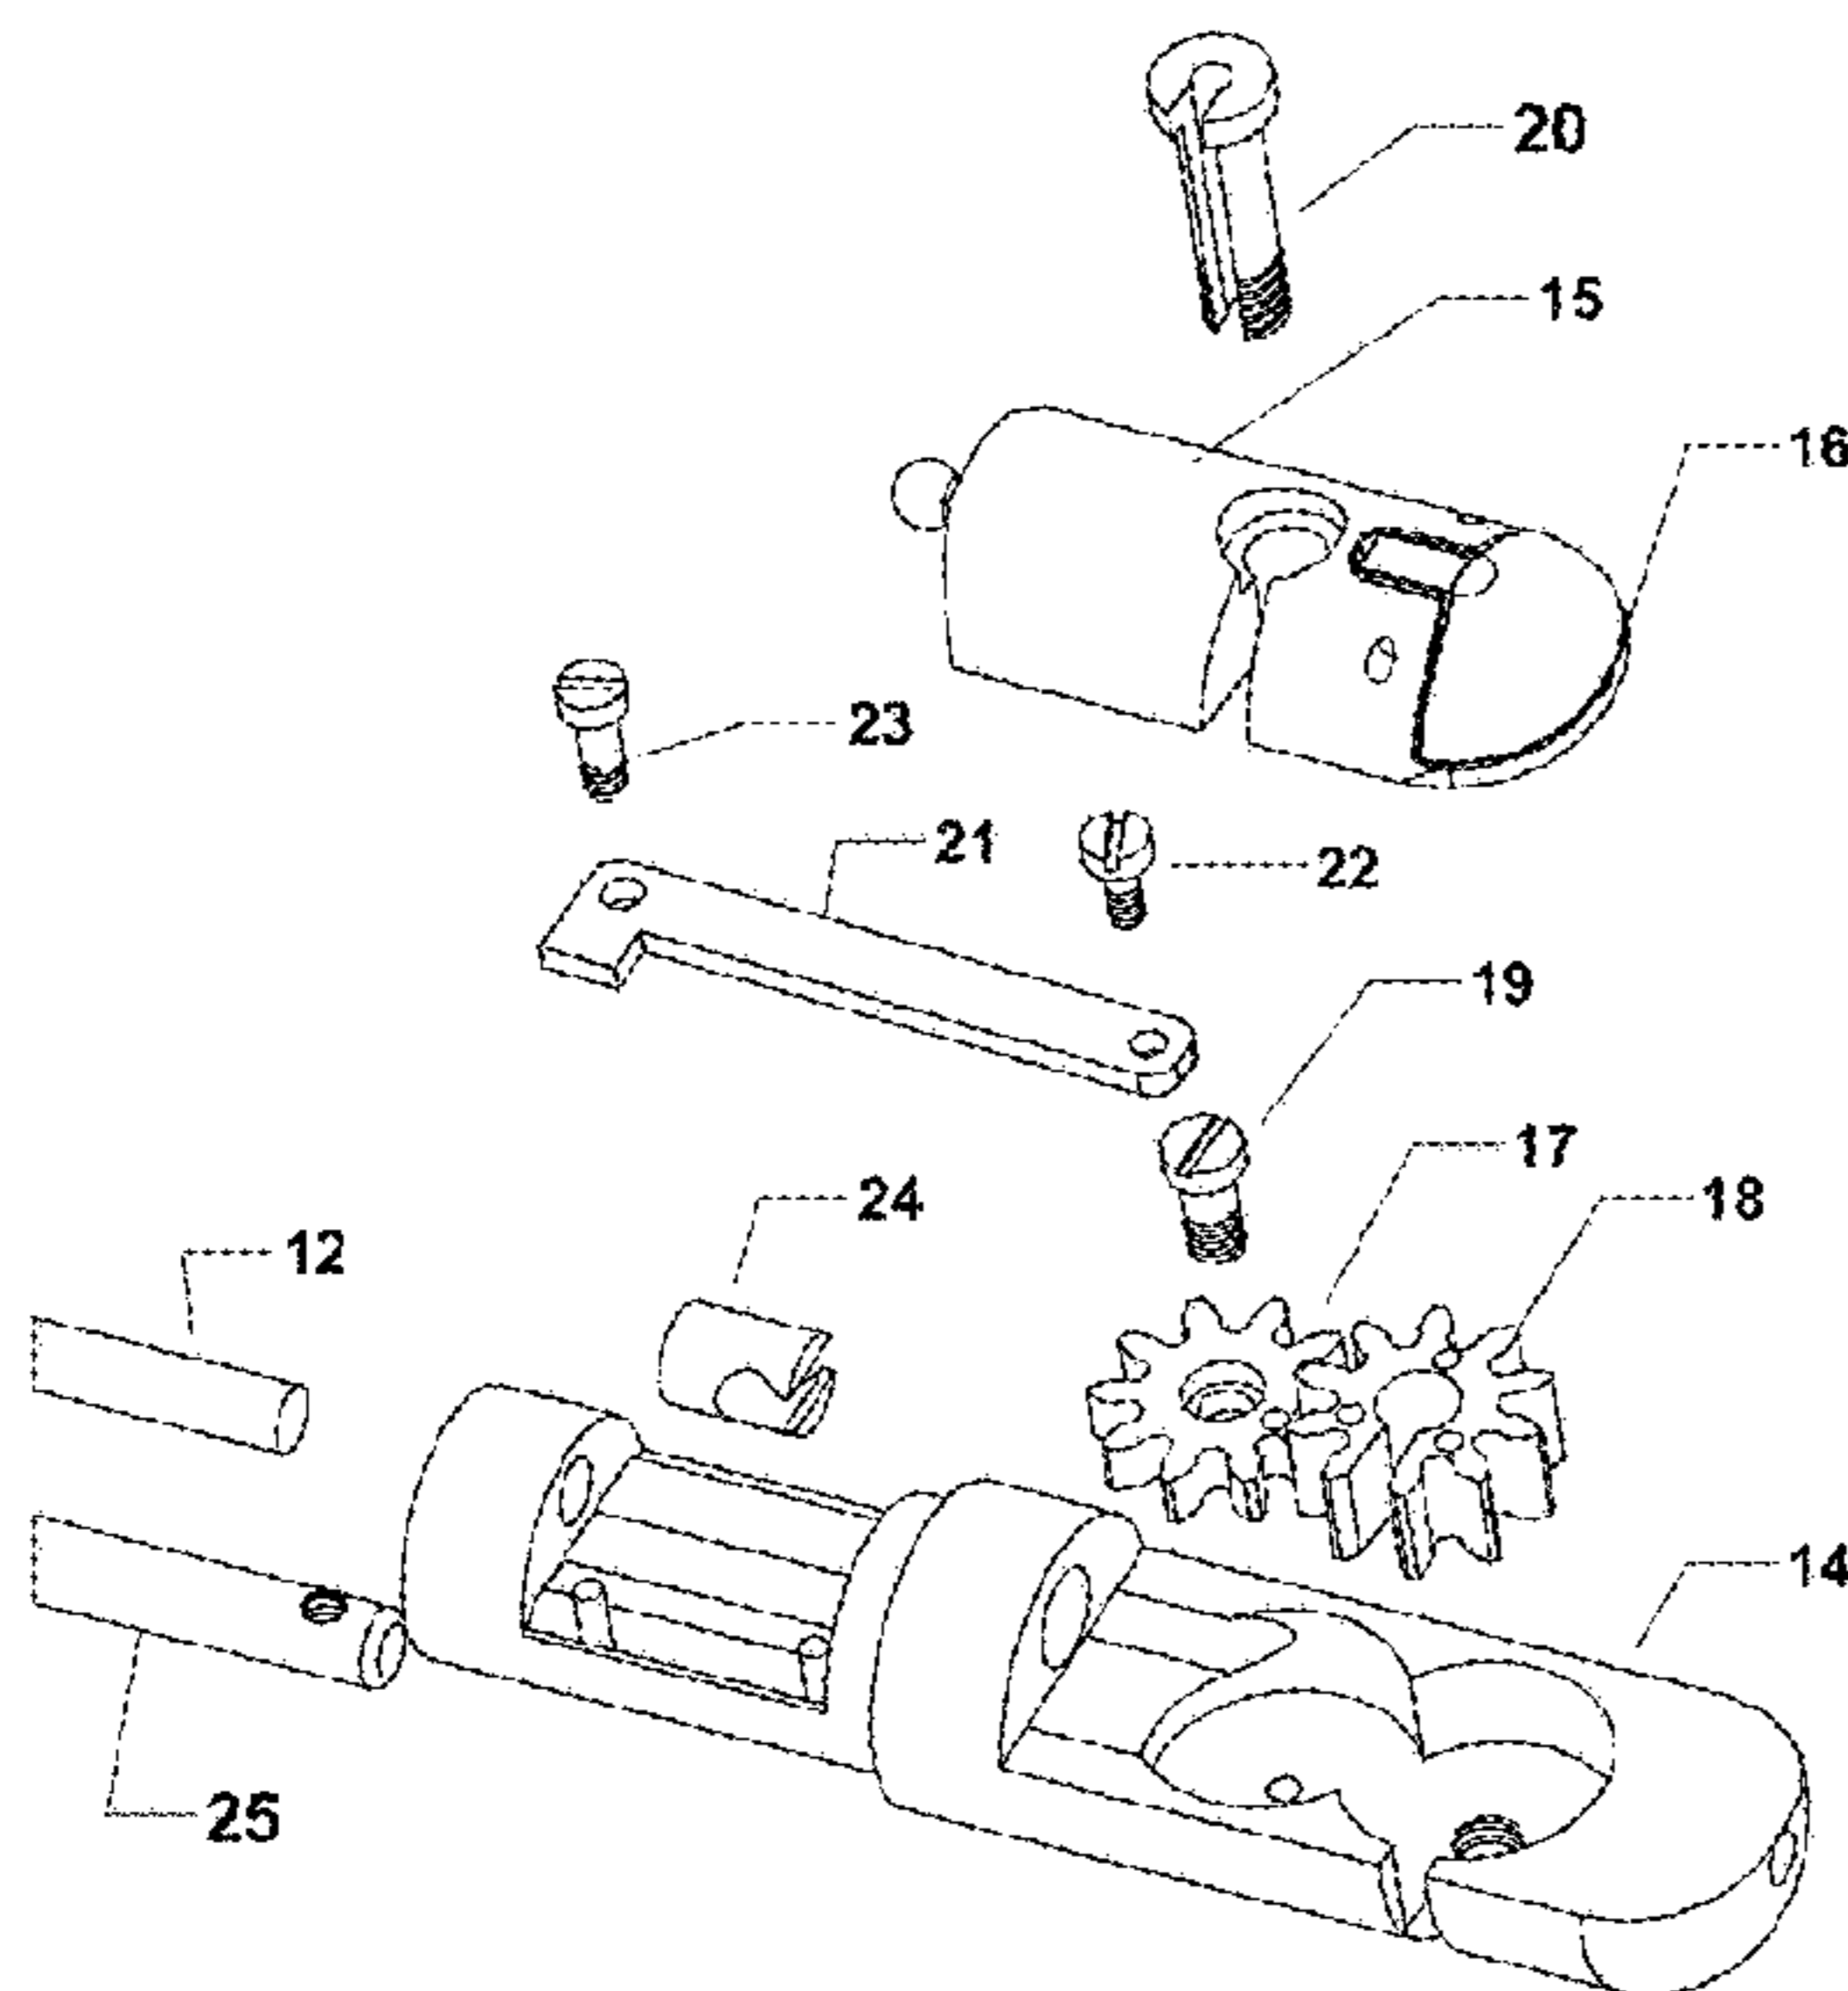

(56)

References Cited

U.S. PATENT DOCUMENTS

5,527,322 A * 6/1996 Klein A61B 17/0057
112/169
5,549,618 A * 8/1996 Fleenor A61B 17/0469
112/169
5,702,407 A * 12/1997 Kaji A61B 17/0469
606/139
5,797,928 A * 8/1998 Kogasaka A61B 17/0469
606/139
6,716,224 B2 * 4/2004 Singhatat A61B 17/0469
289/17
7,833,237 B2 * 11/2010 Sauer A61B 17/0467
606/139
8,038,689 B2 * 10/2011 Kawai A61B 17/0469
606/139
9,107,657 B2 * 8/2015 Uchida A61B 17/0469
9,194,468 B1 * 11/2015 Fan F16H 21/28
9,427,226 B2 * 8/2016 Martin A61B 17/0469
2014/0276979 A1 * 9/2014 Sauer A61B 17/0469
606/144

* cited by examiner

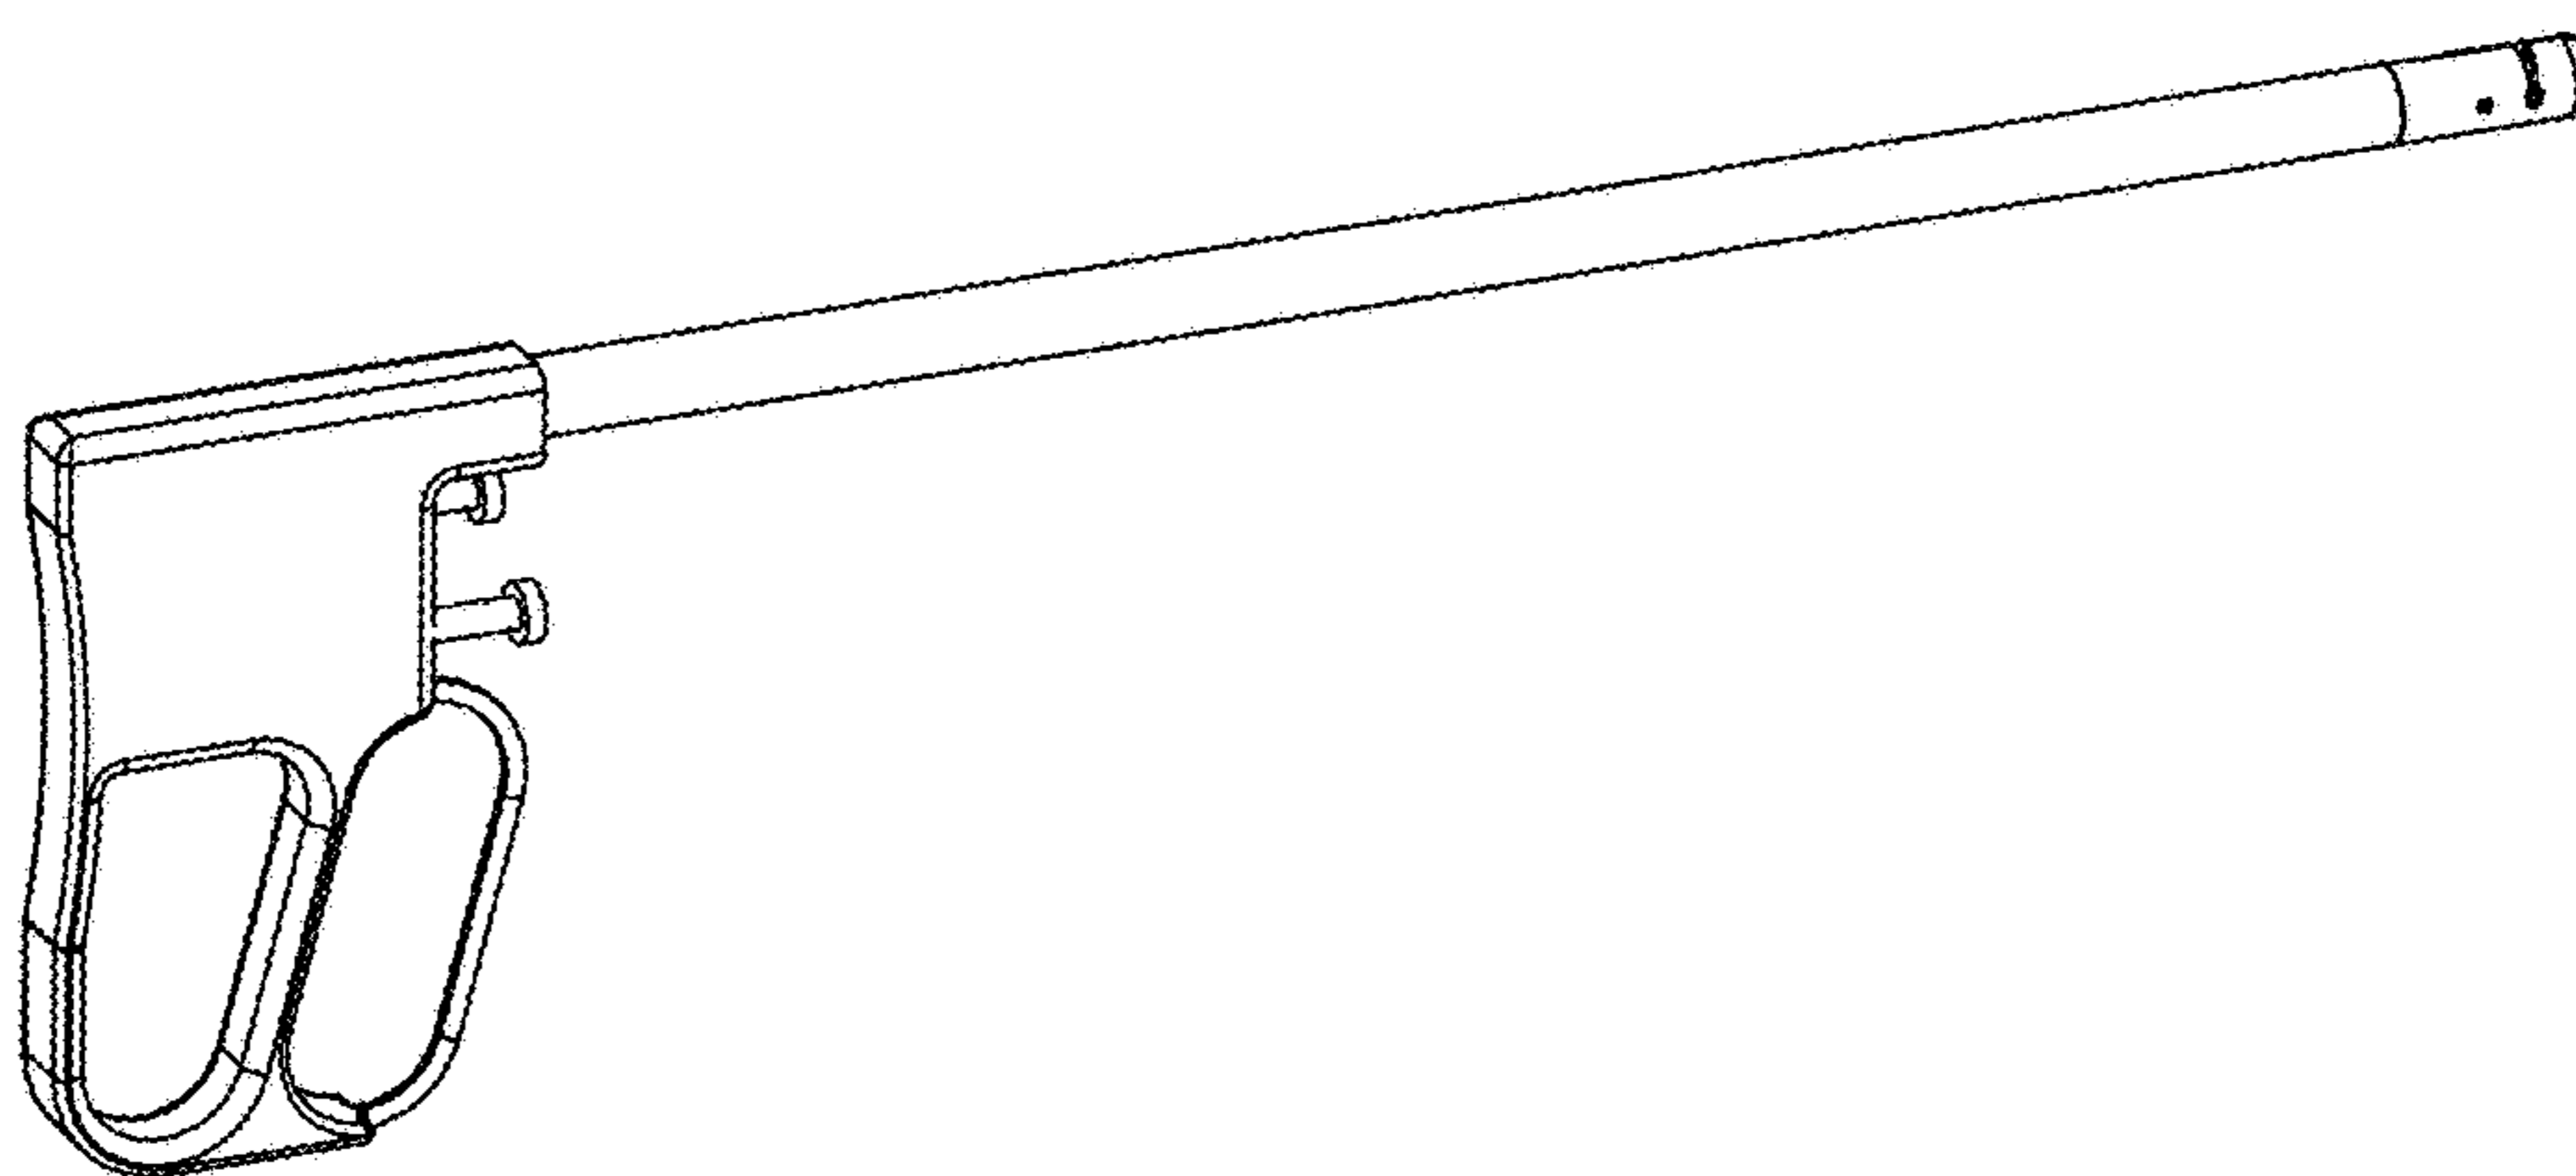


Fig. 1

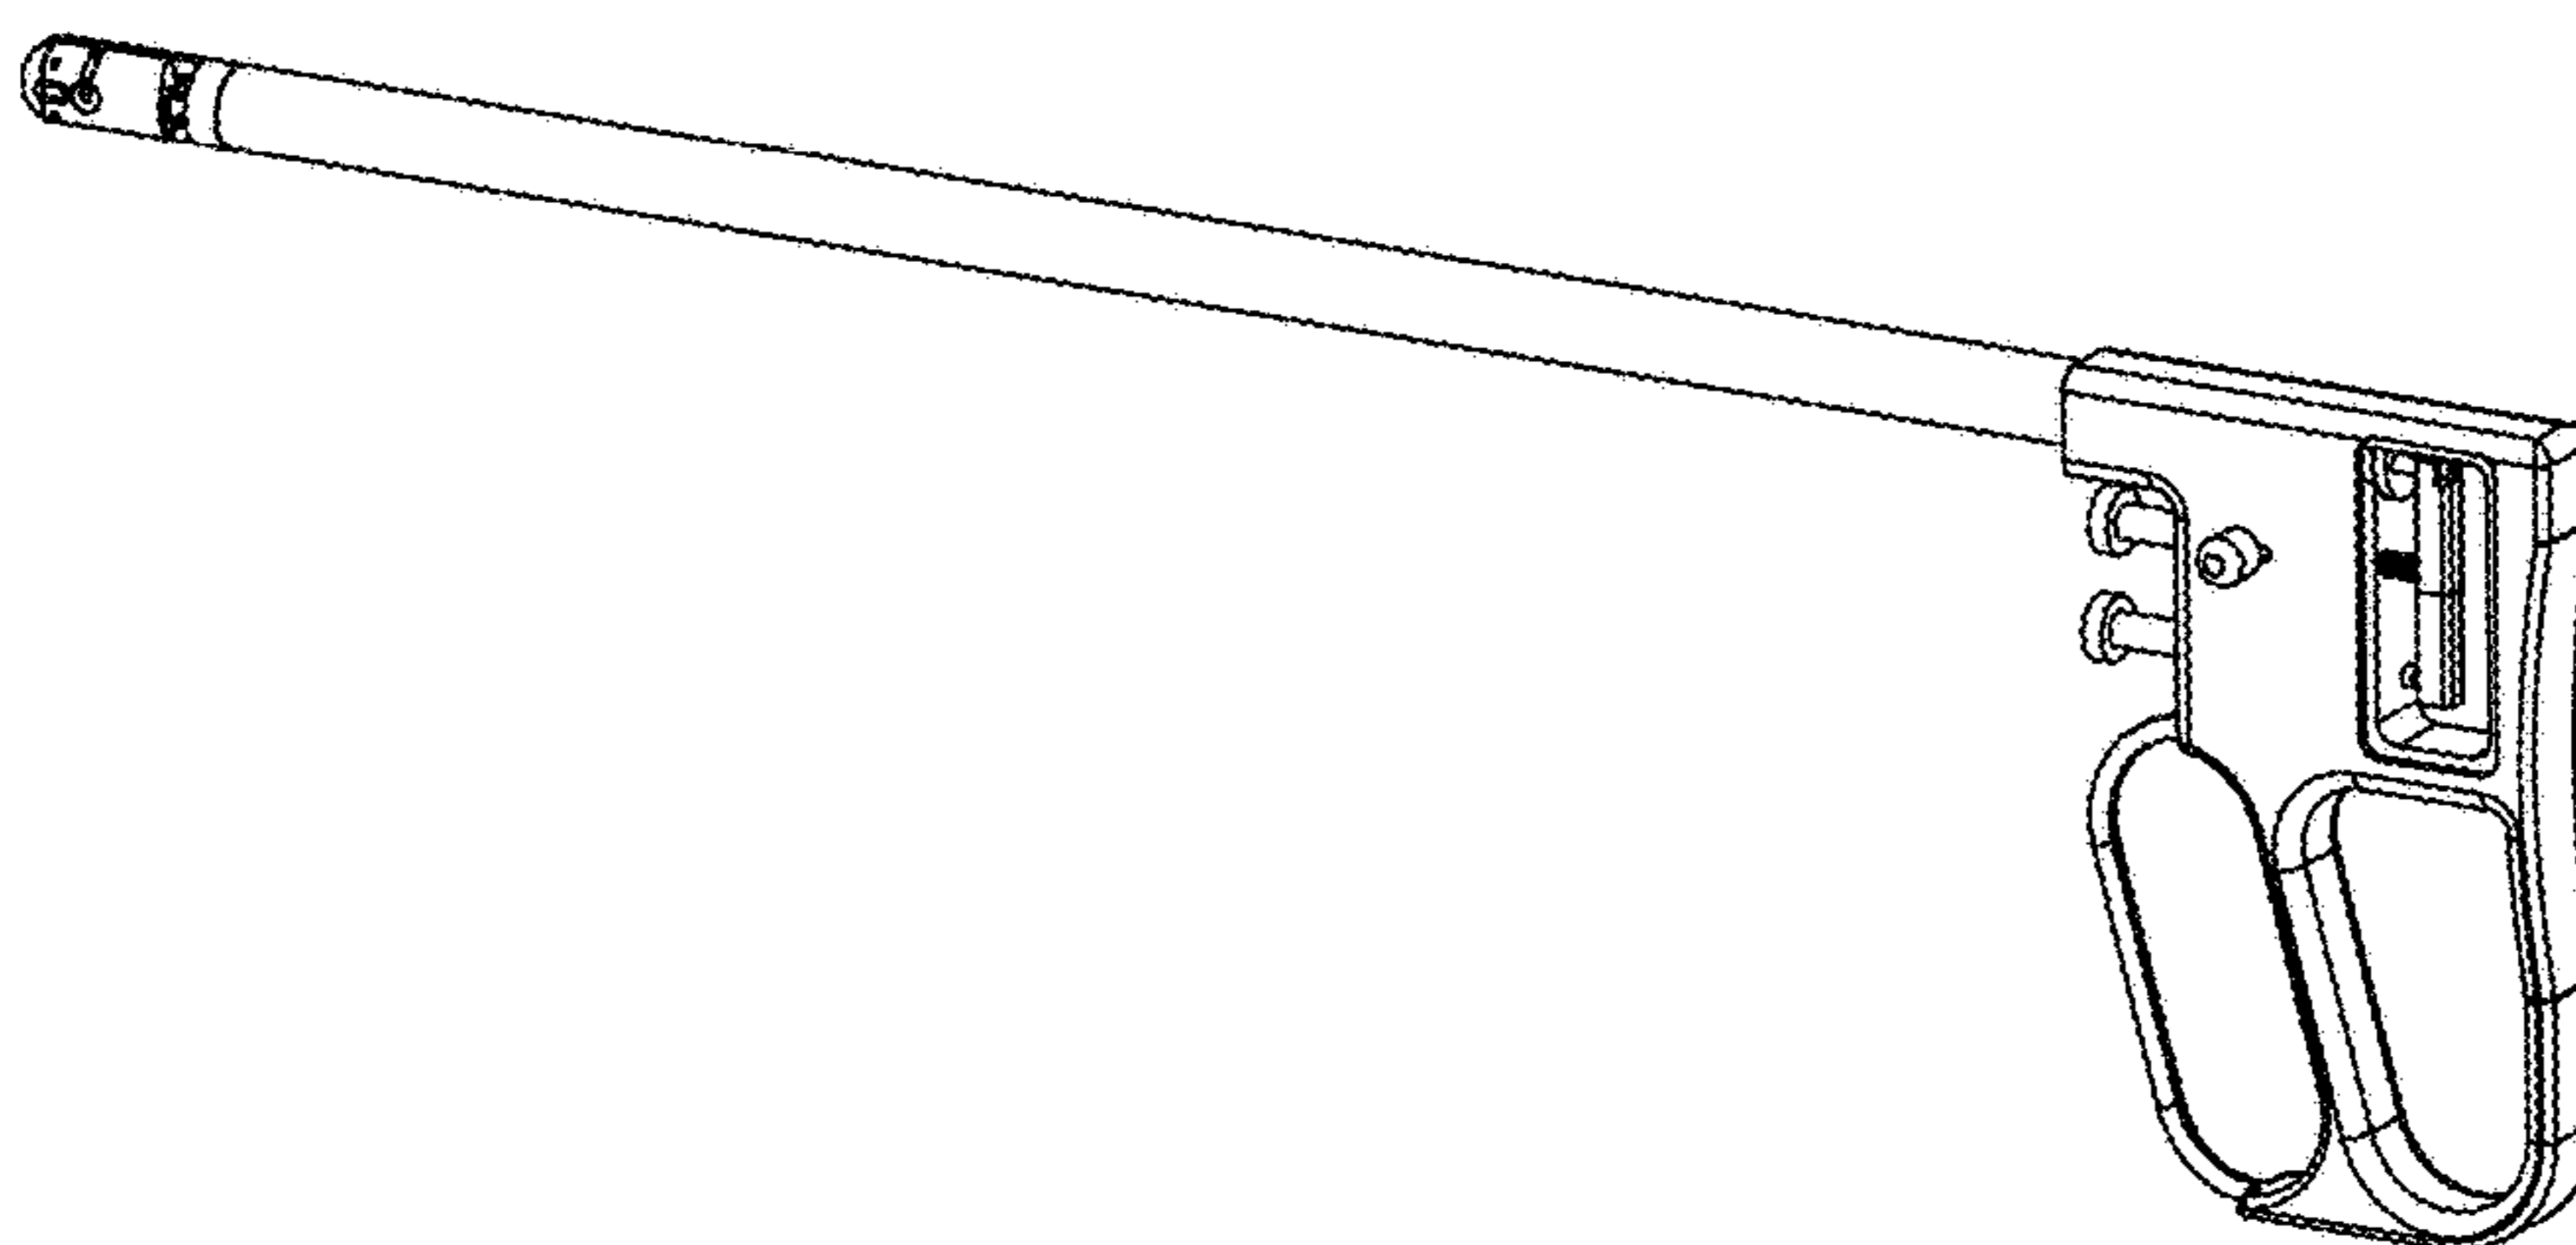


Fig. 2

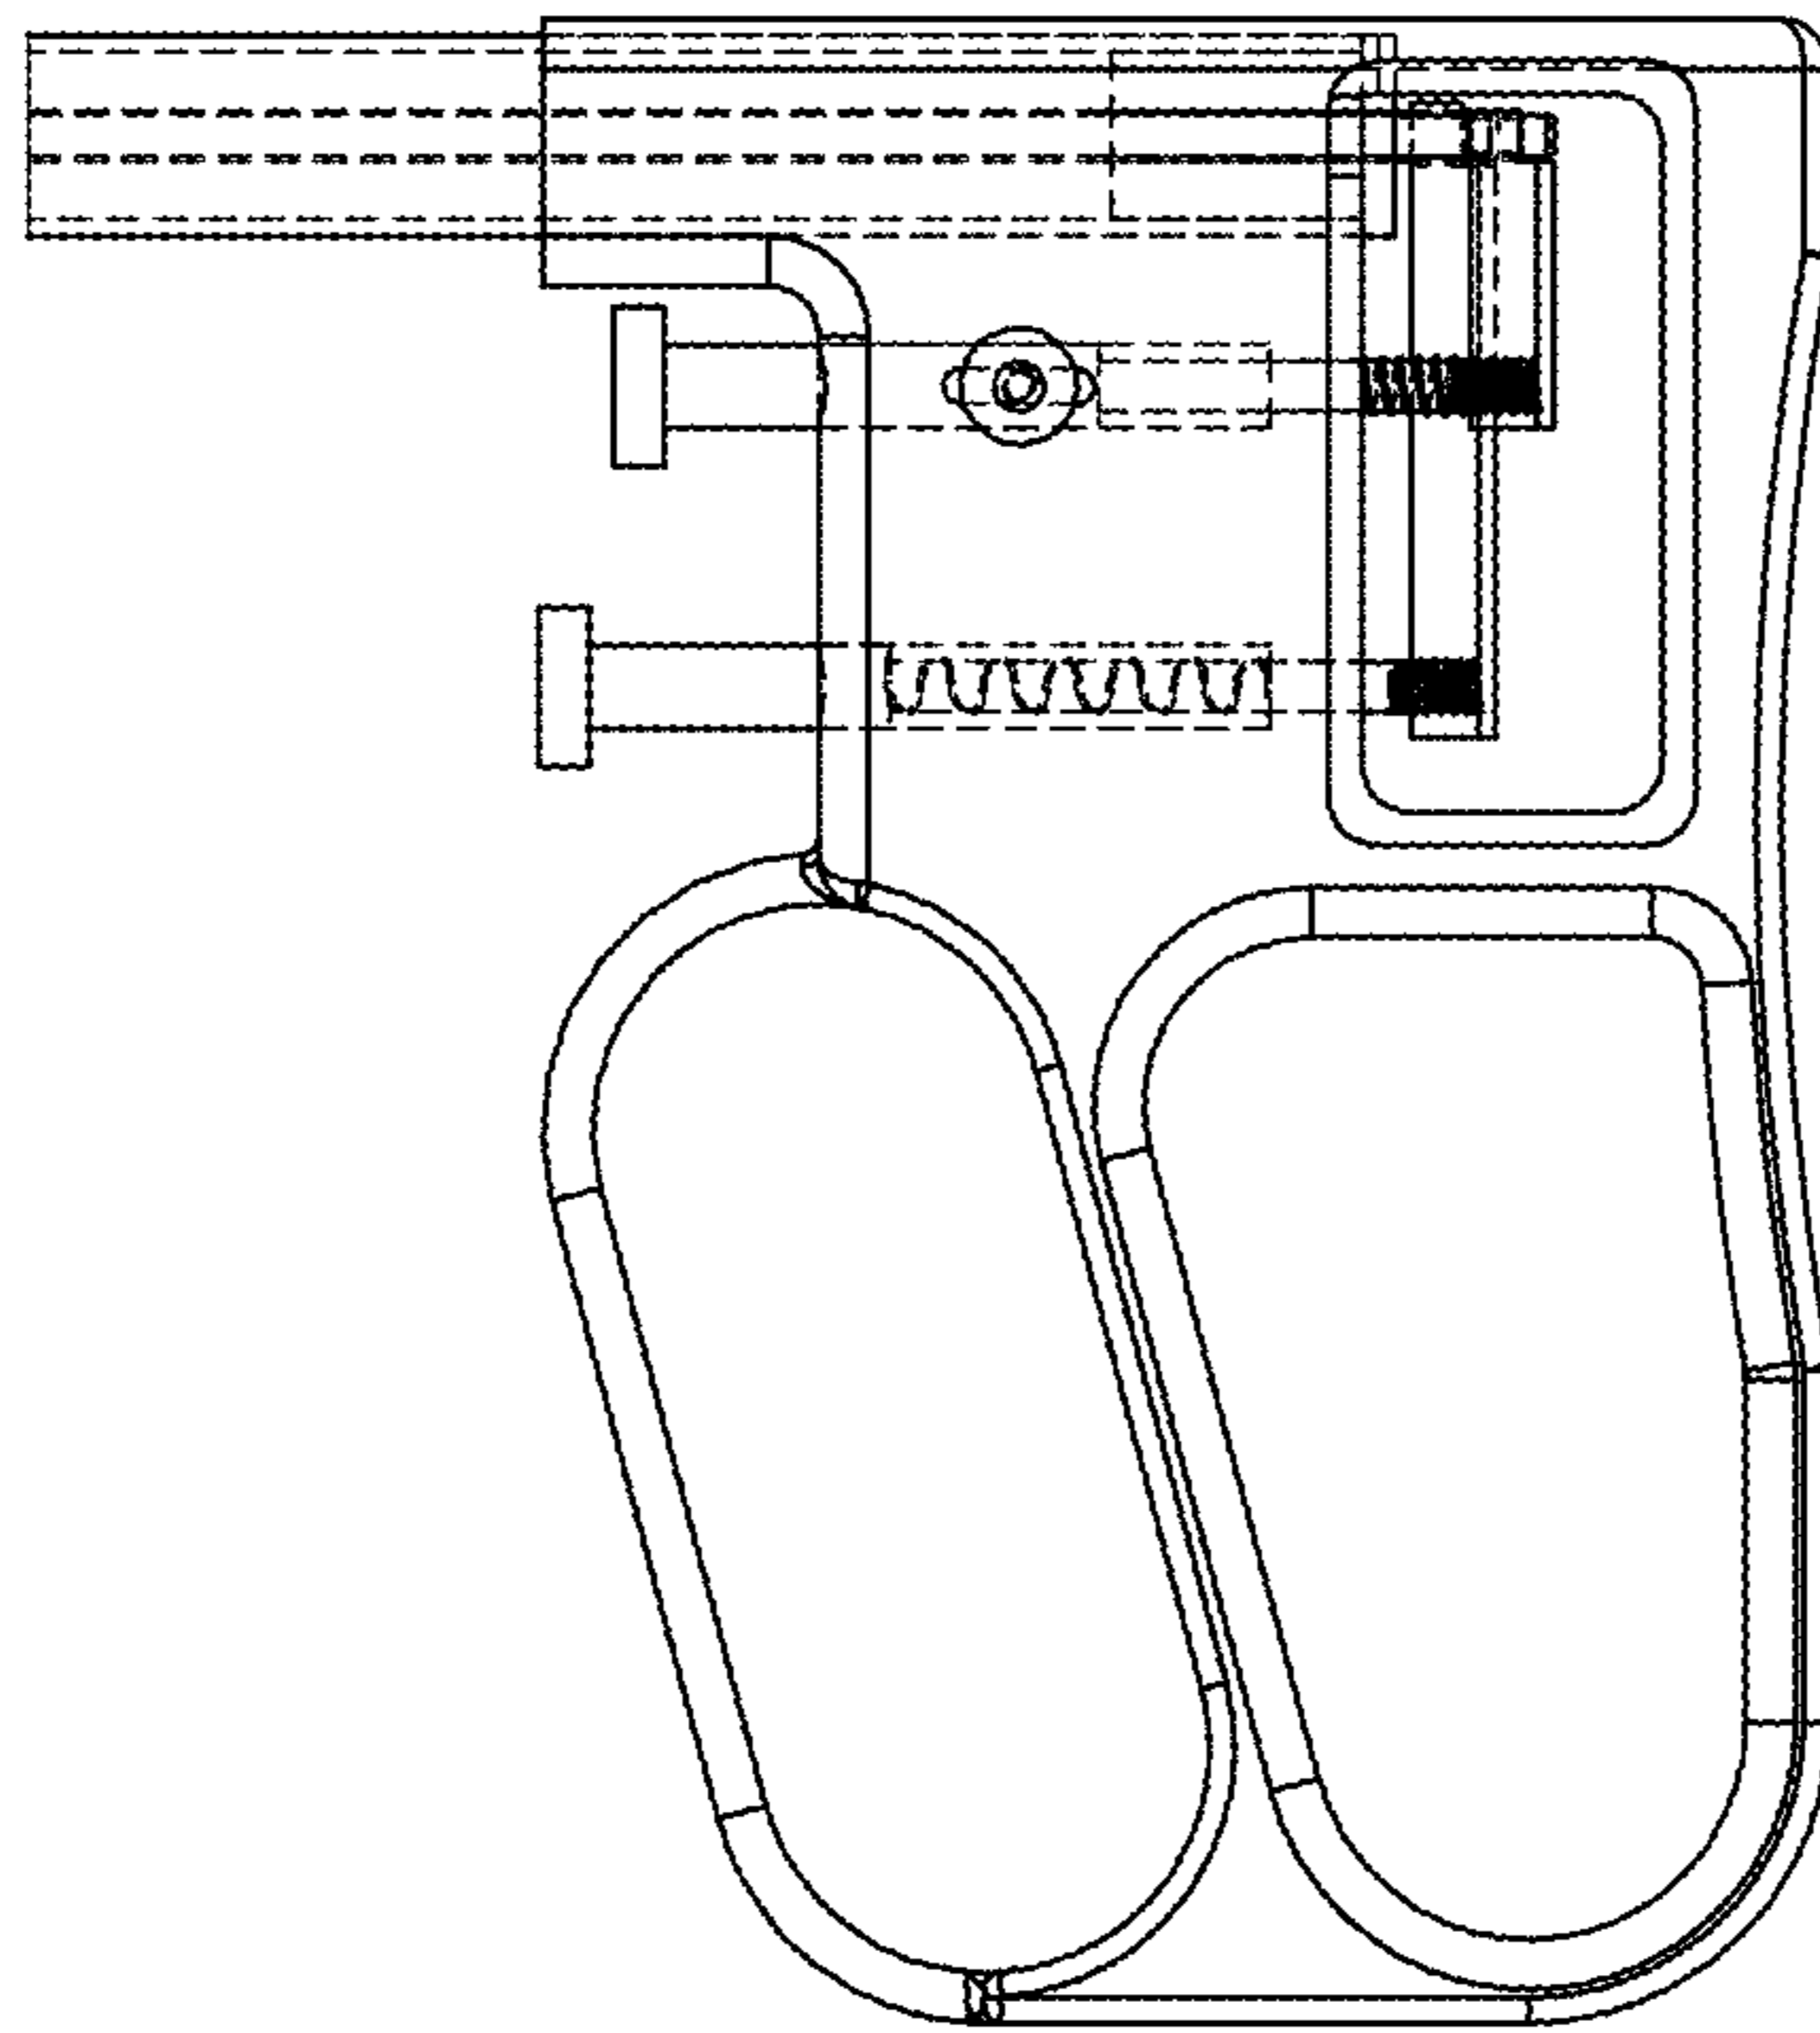


Fig. 3

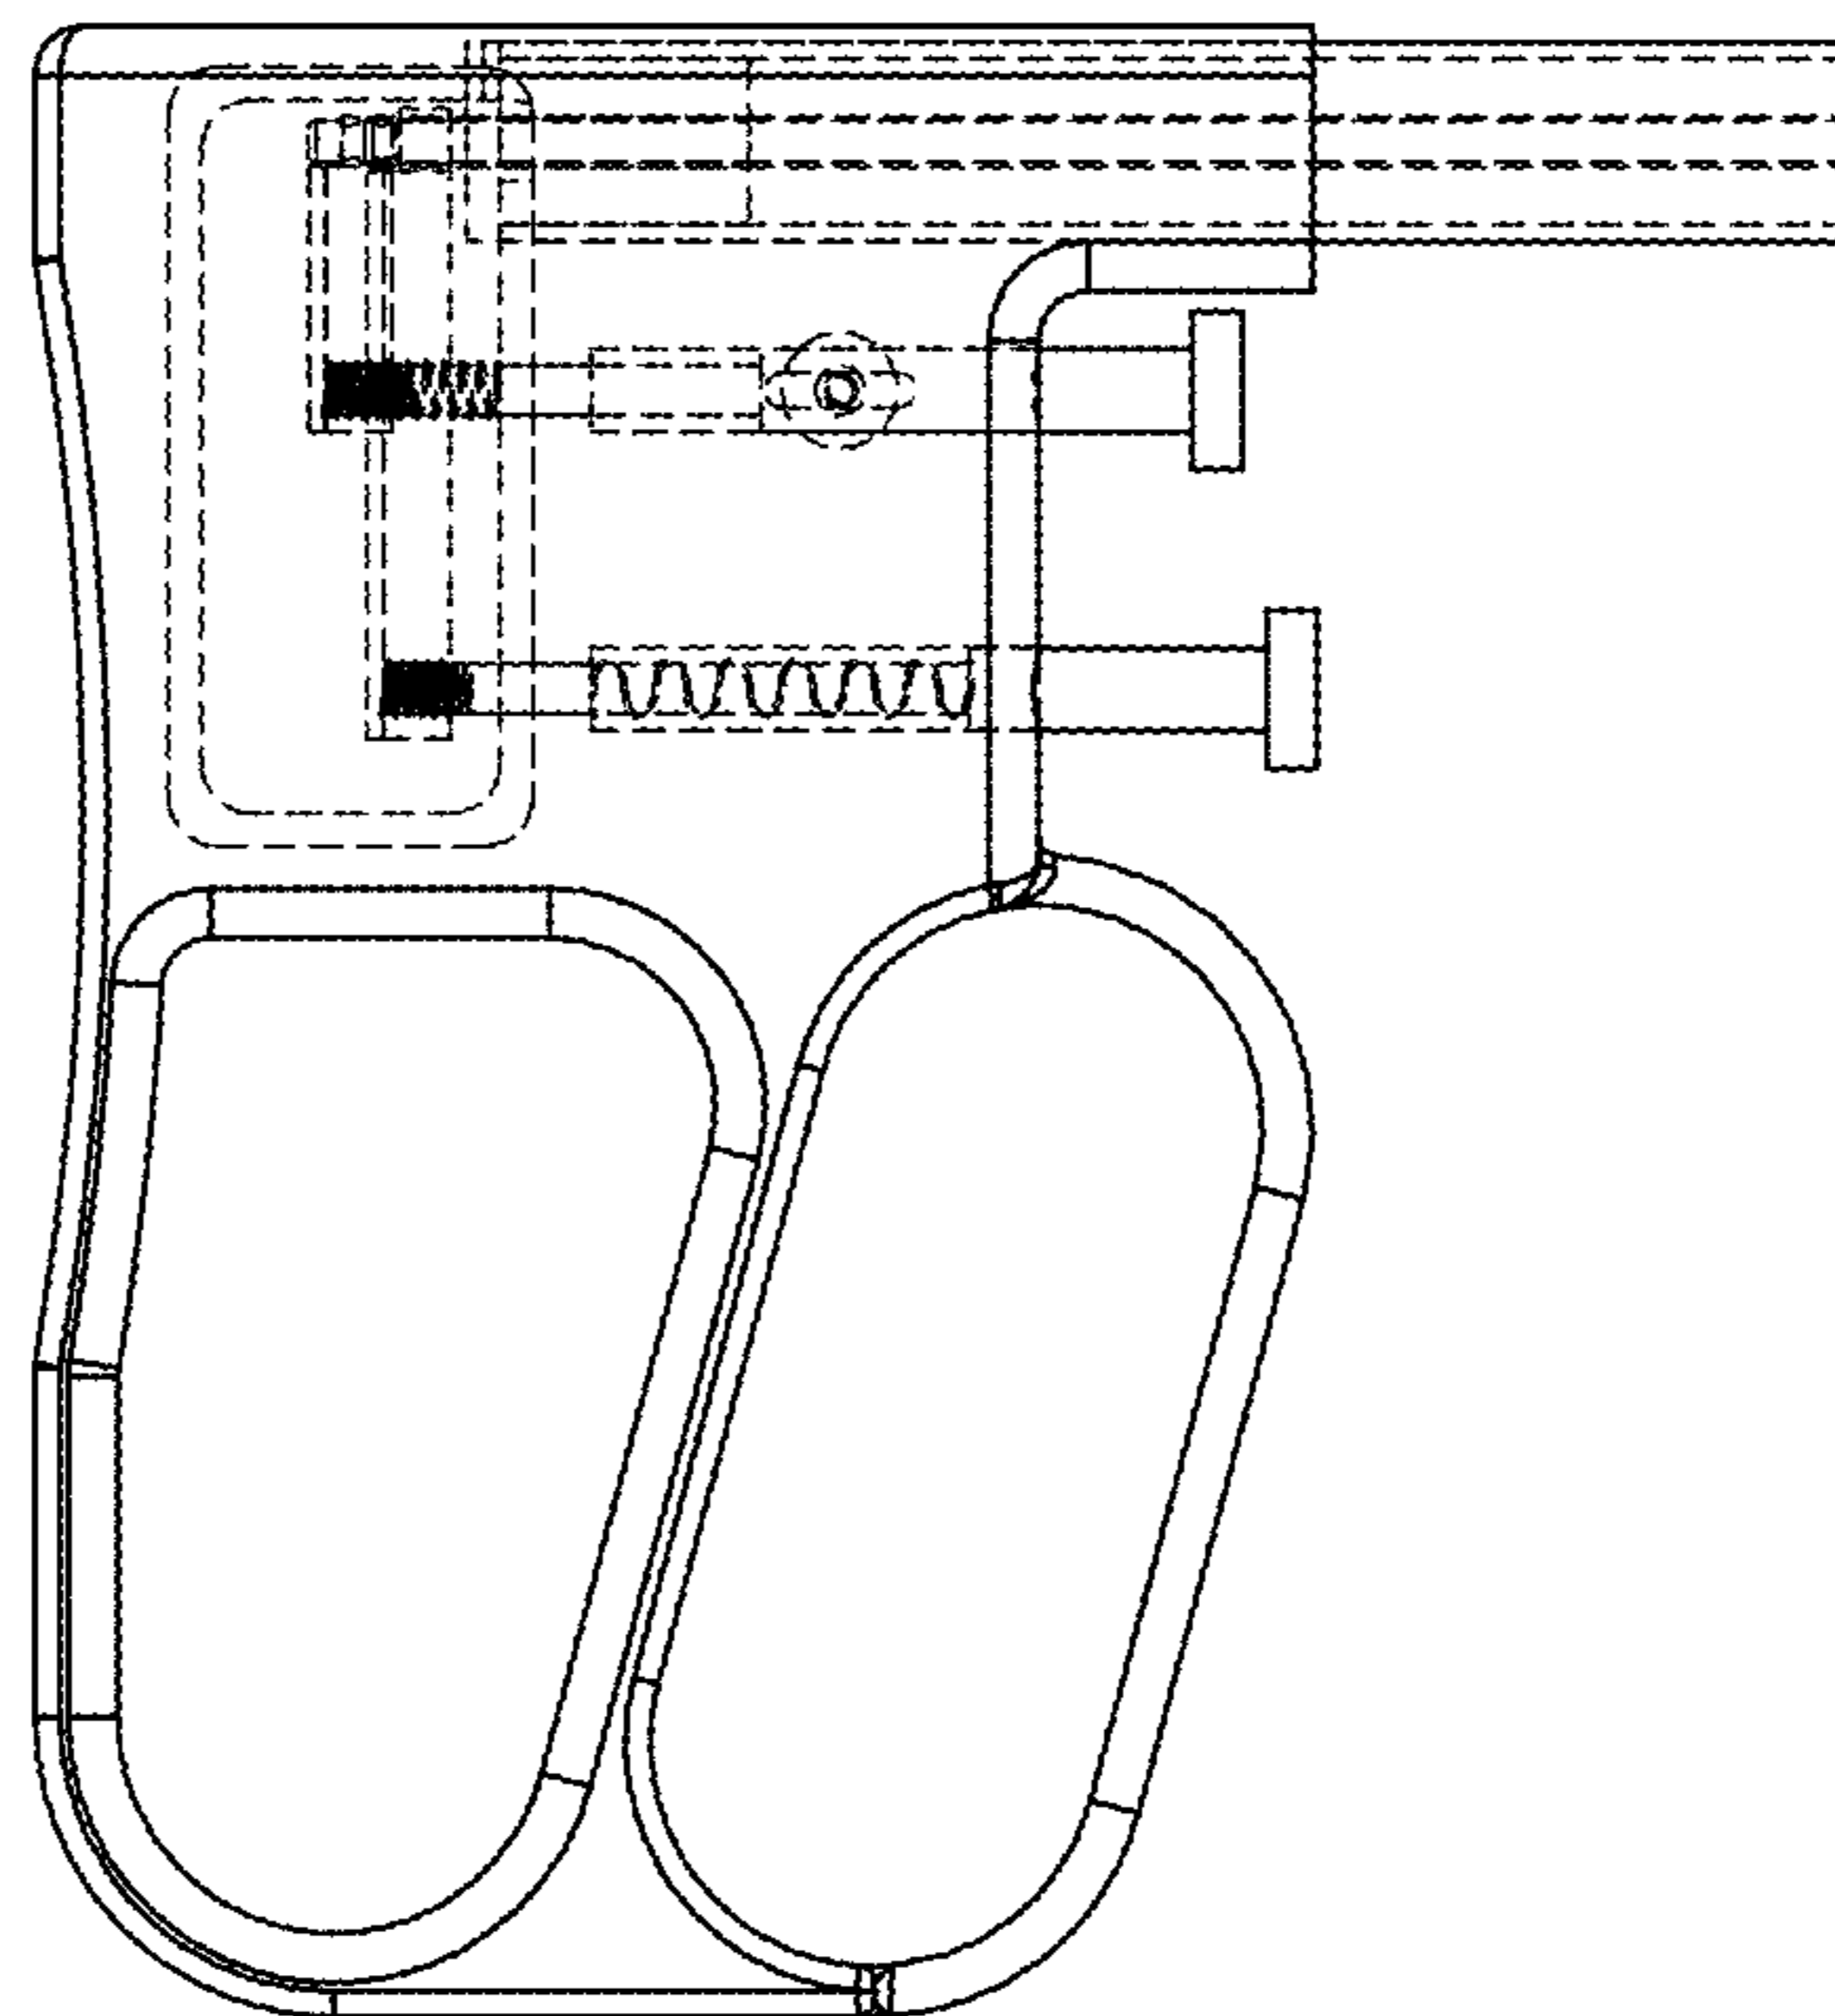


Fig. 4

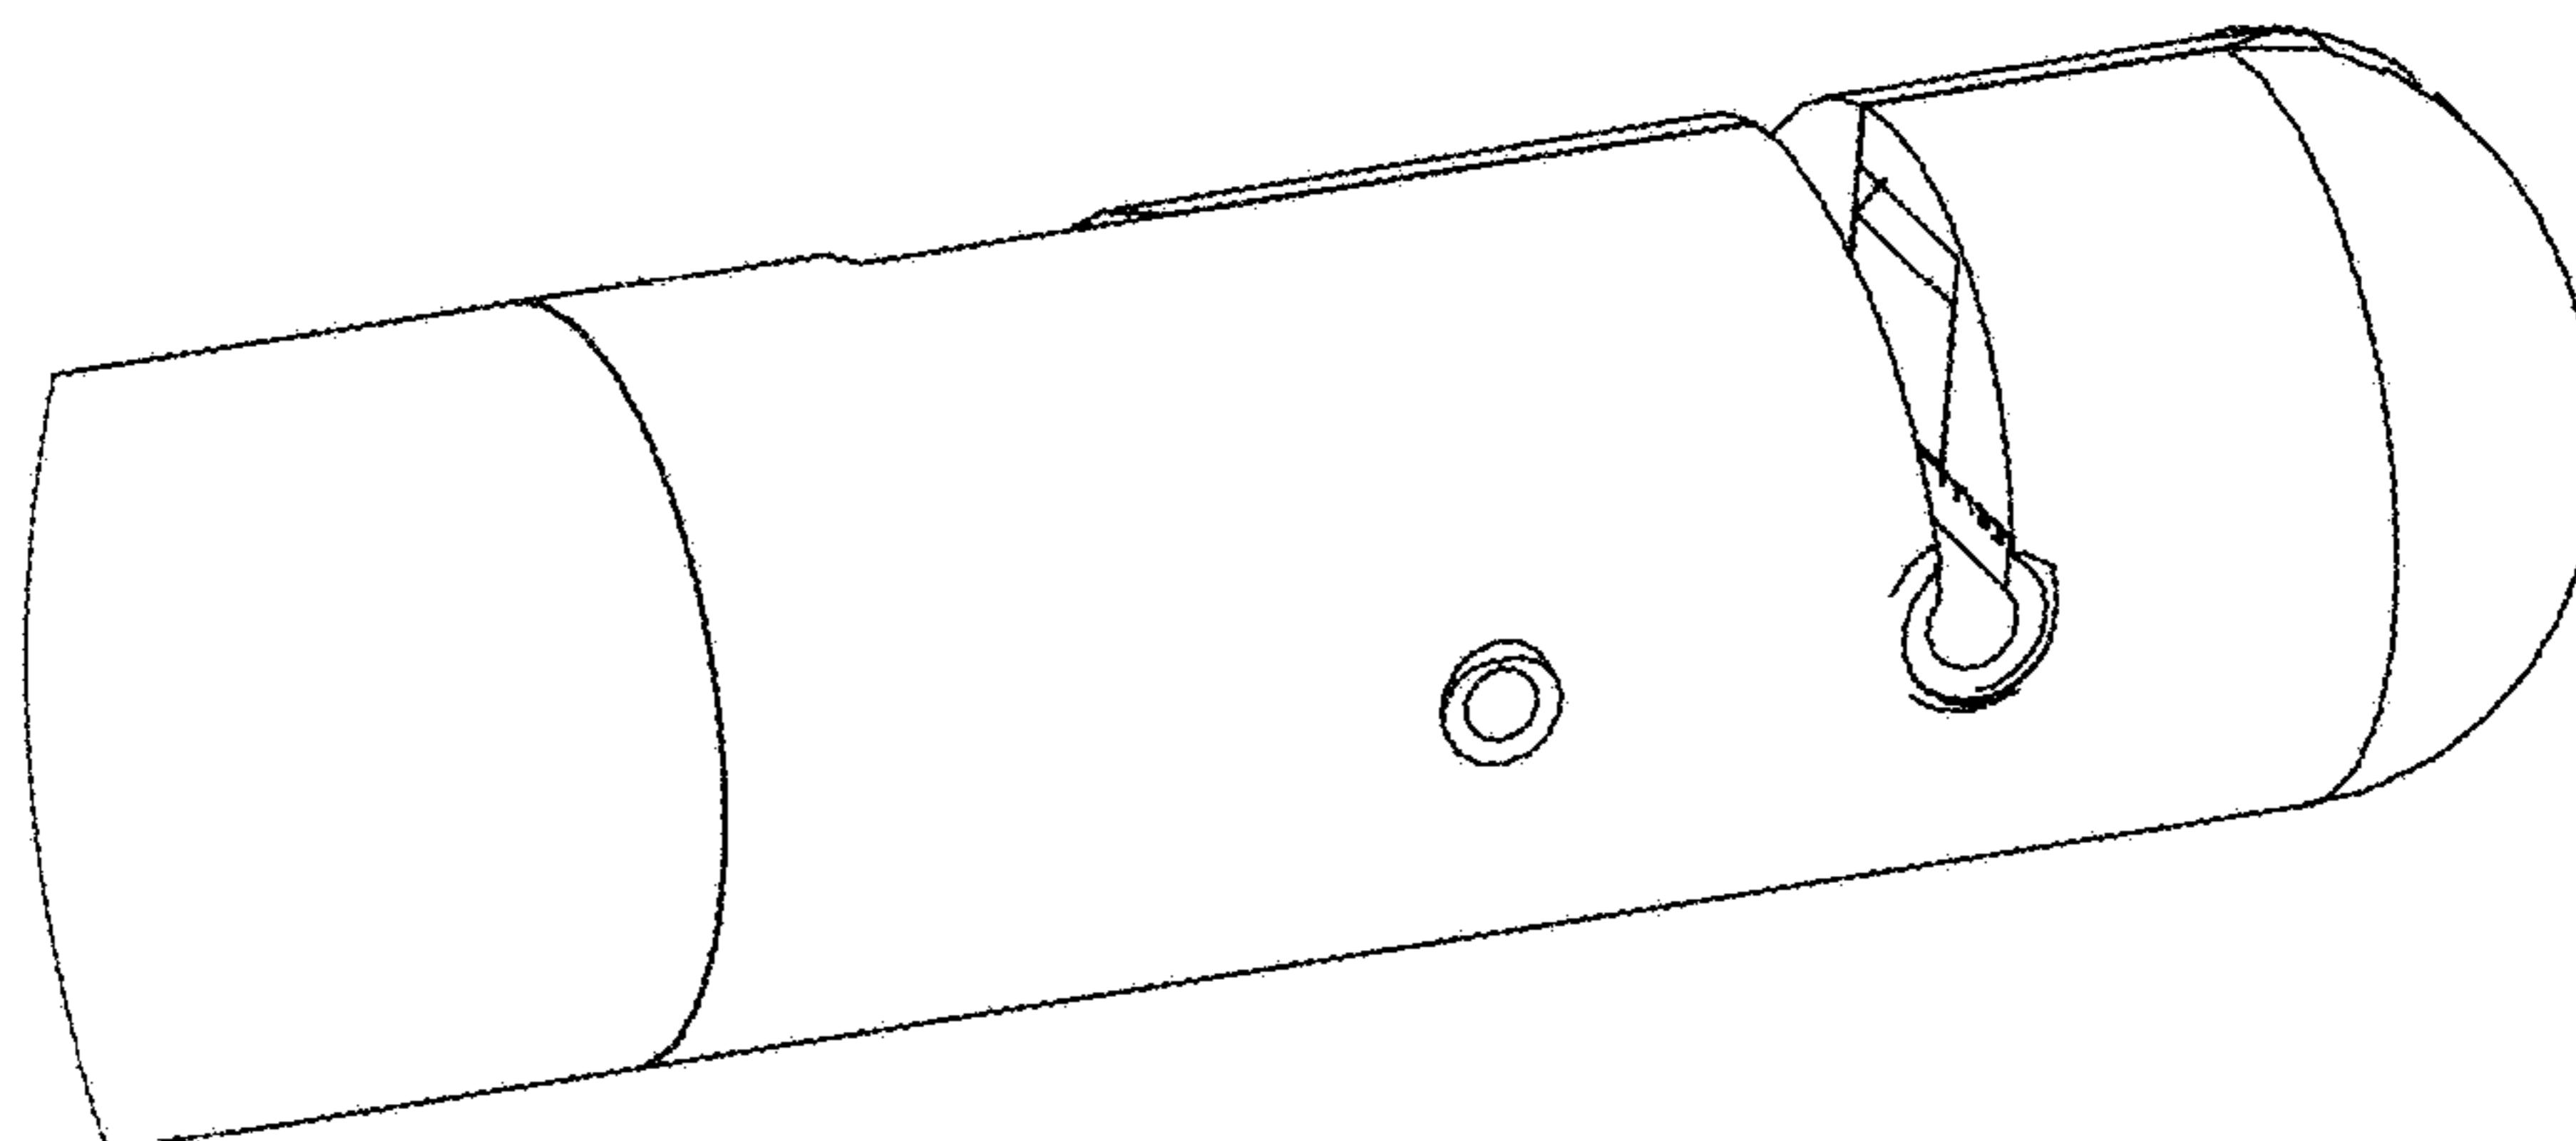


Fig. 5

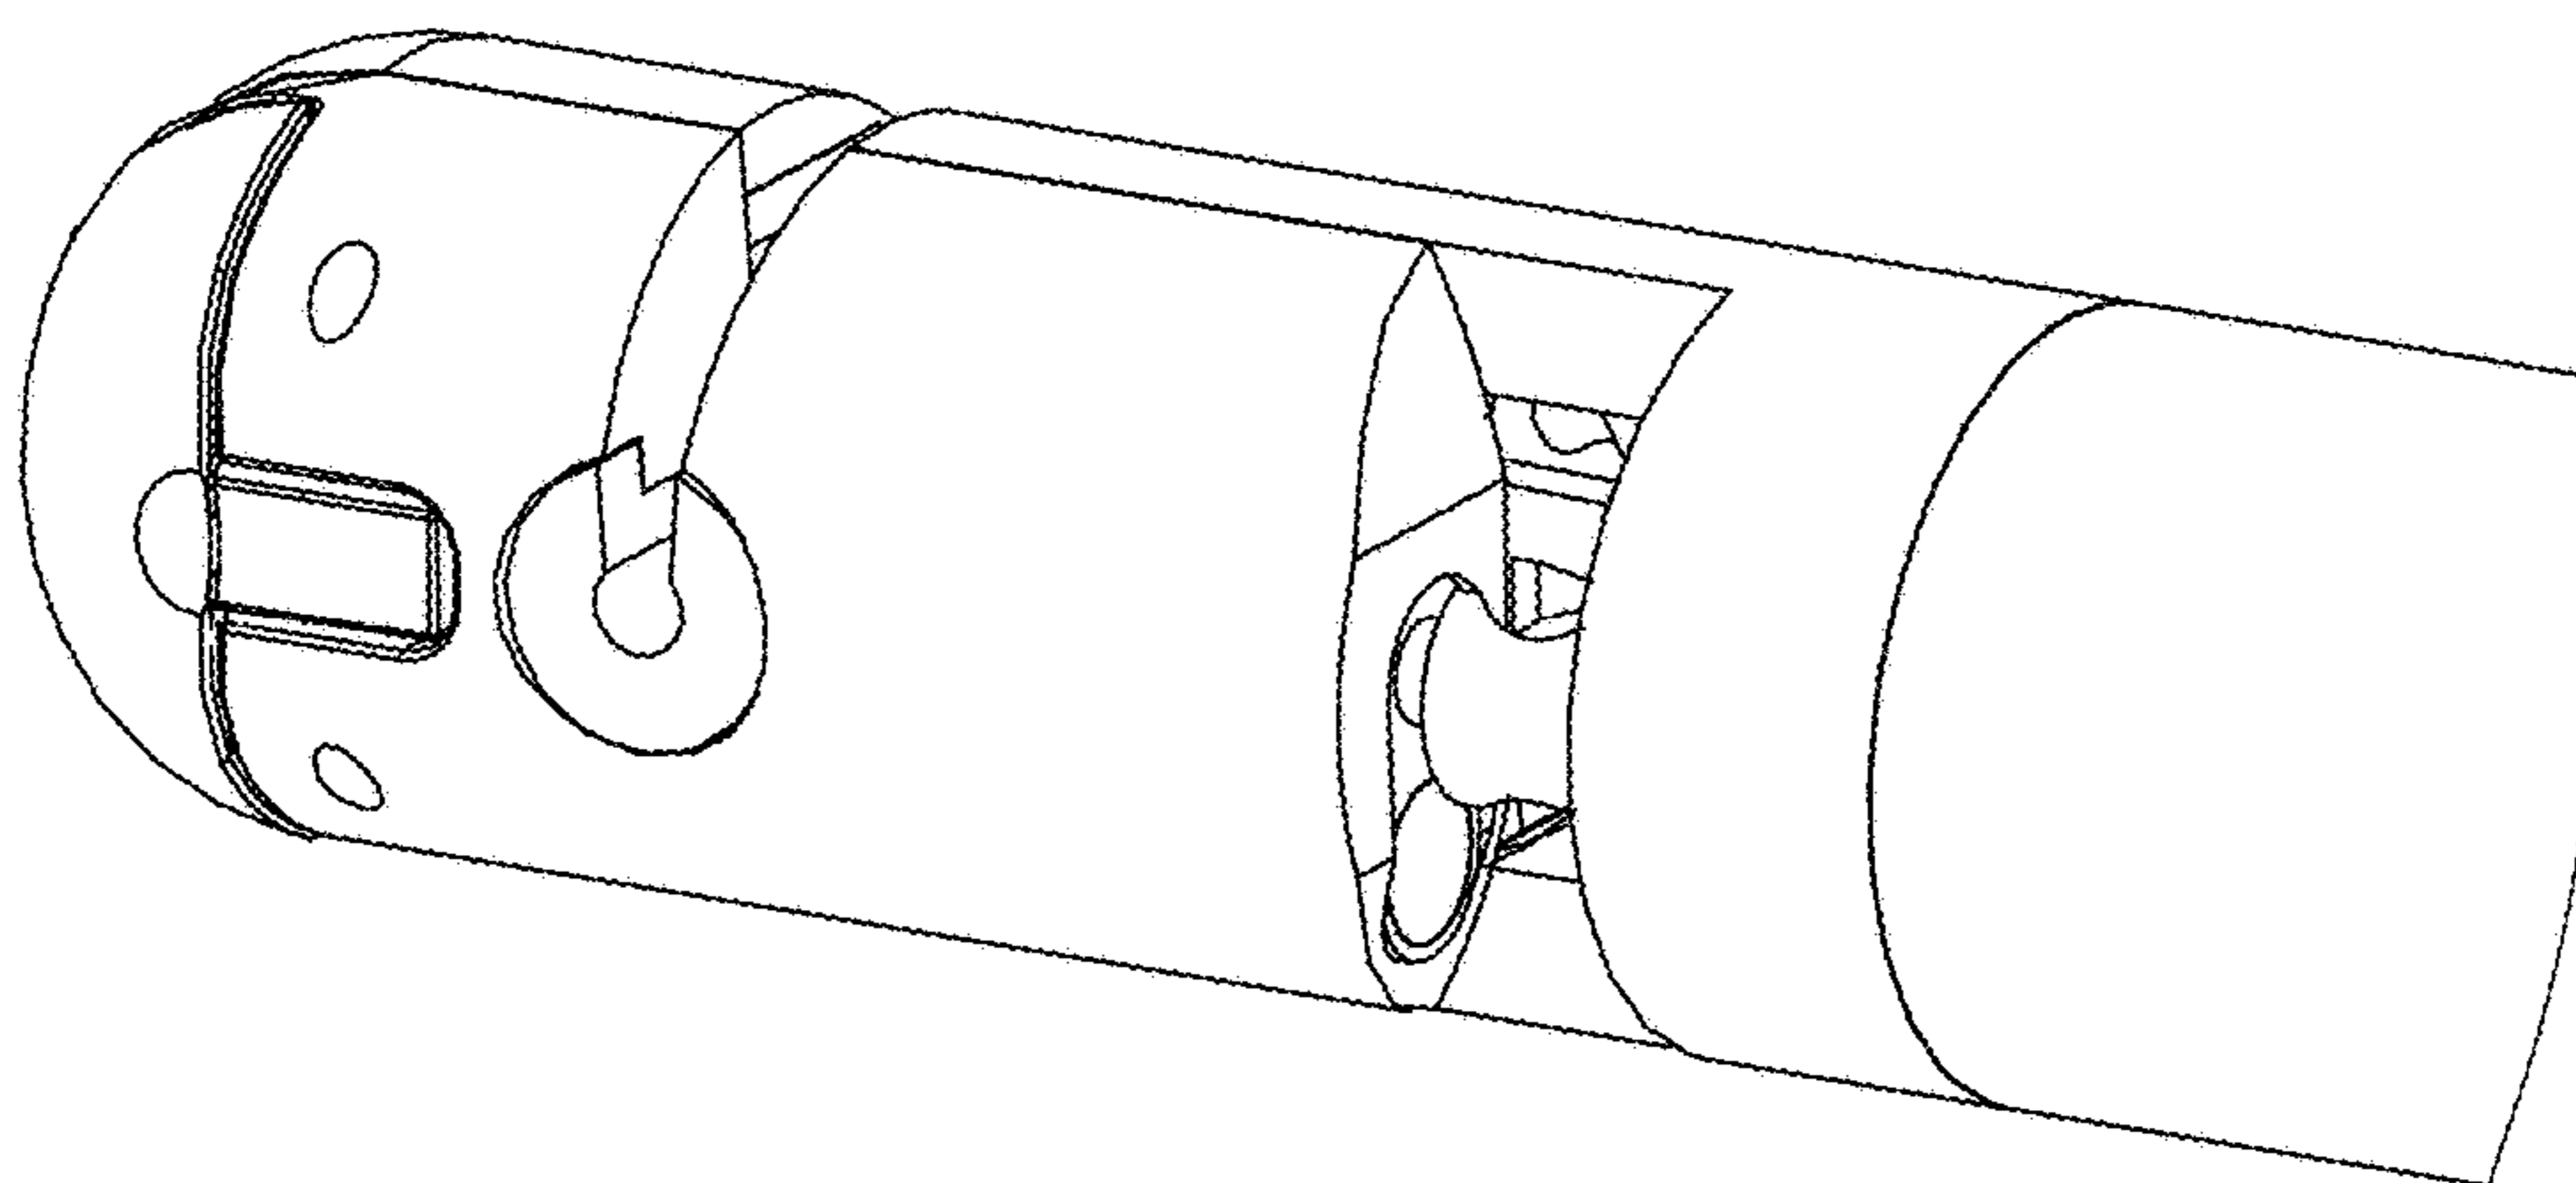


Fig. 6

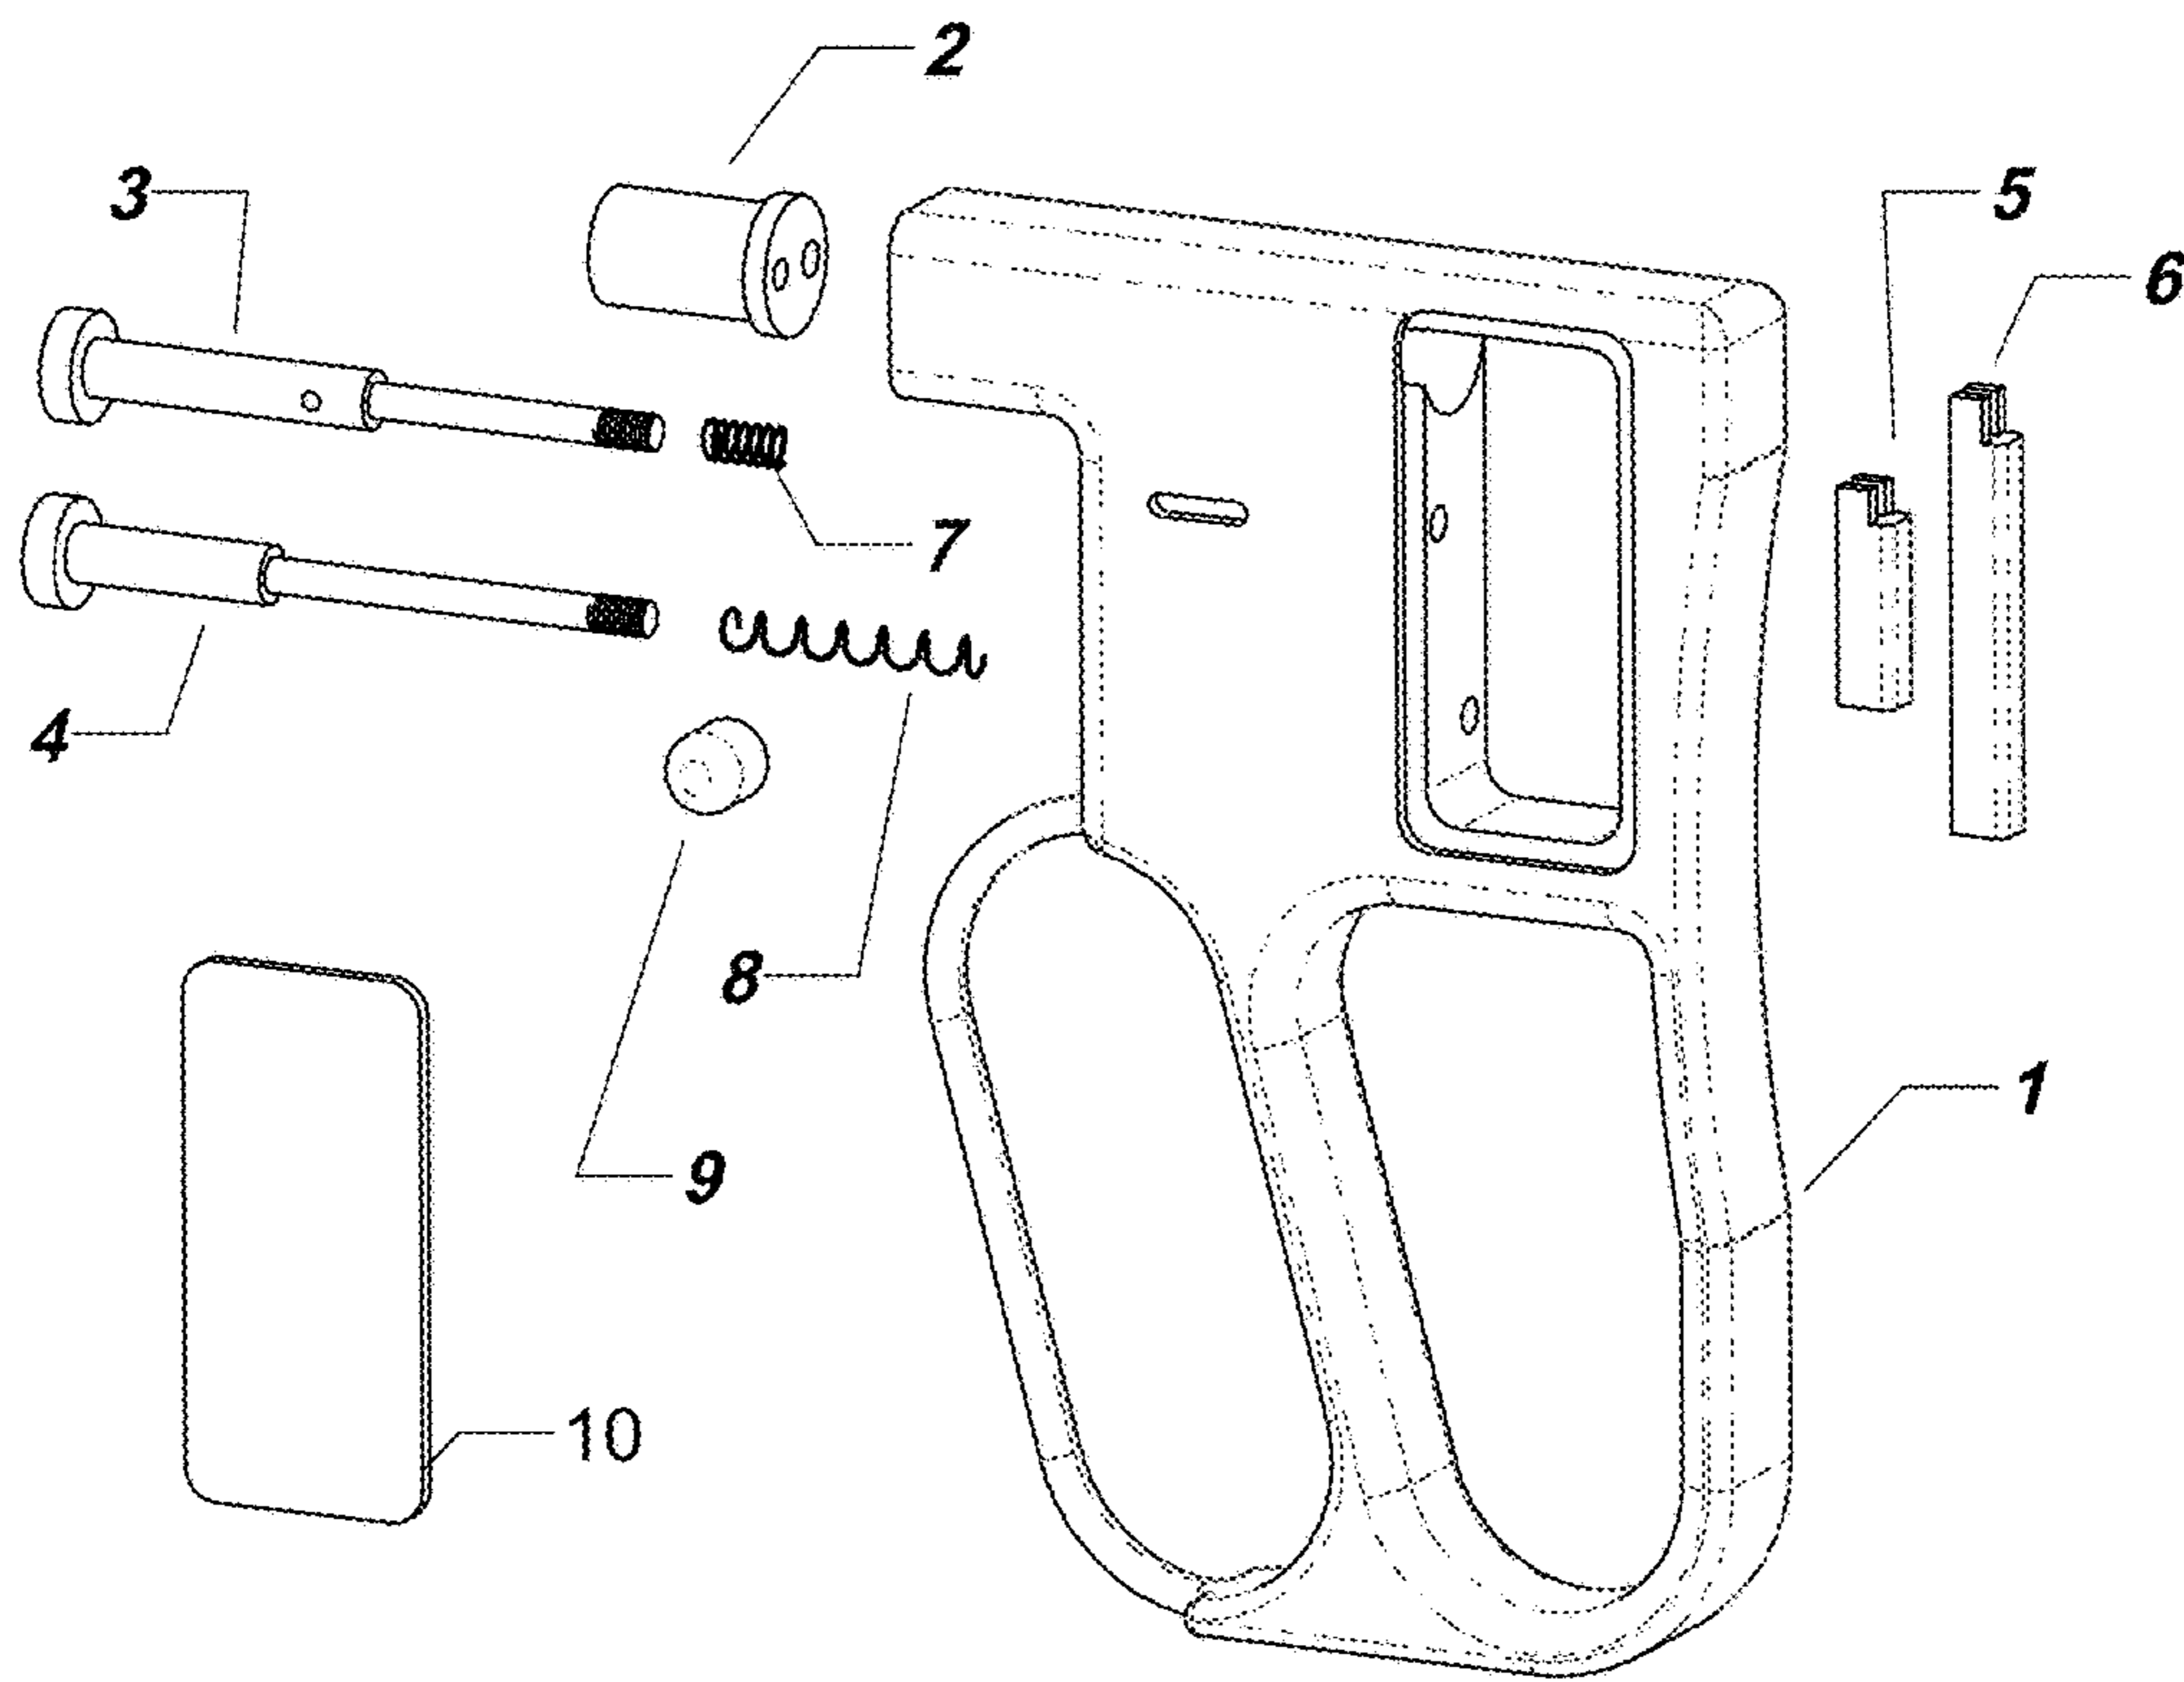


Fig. 7

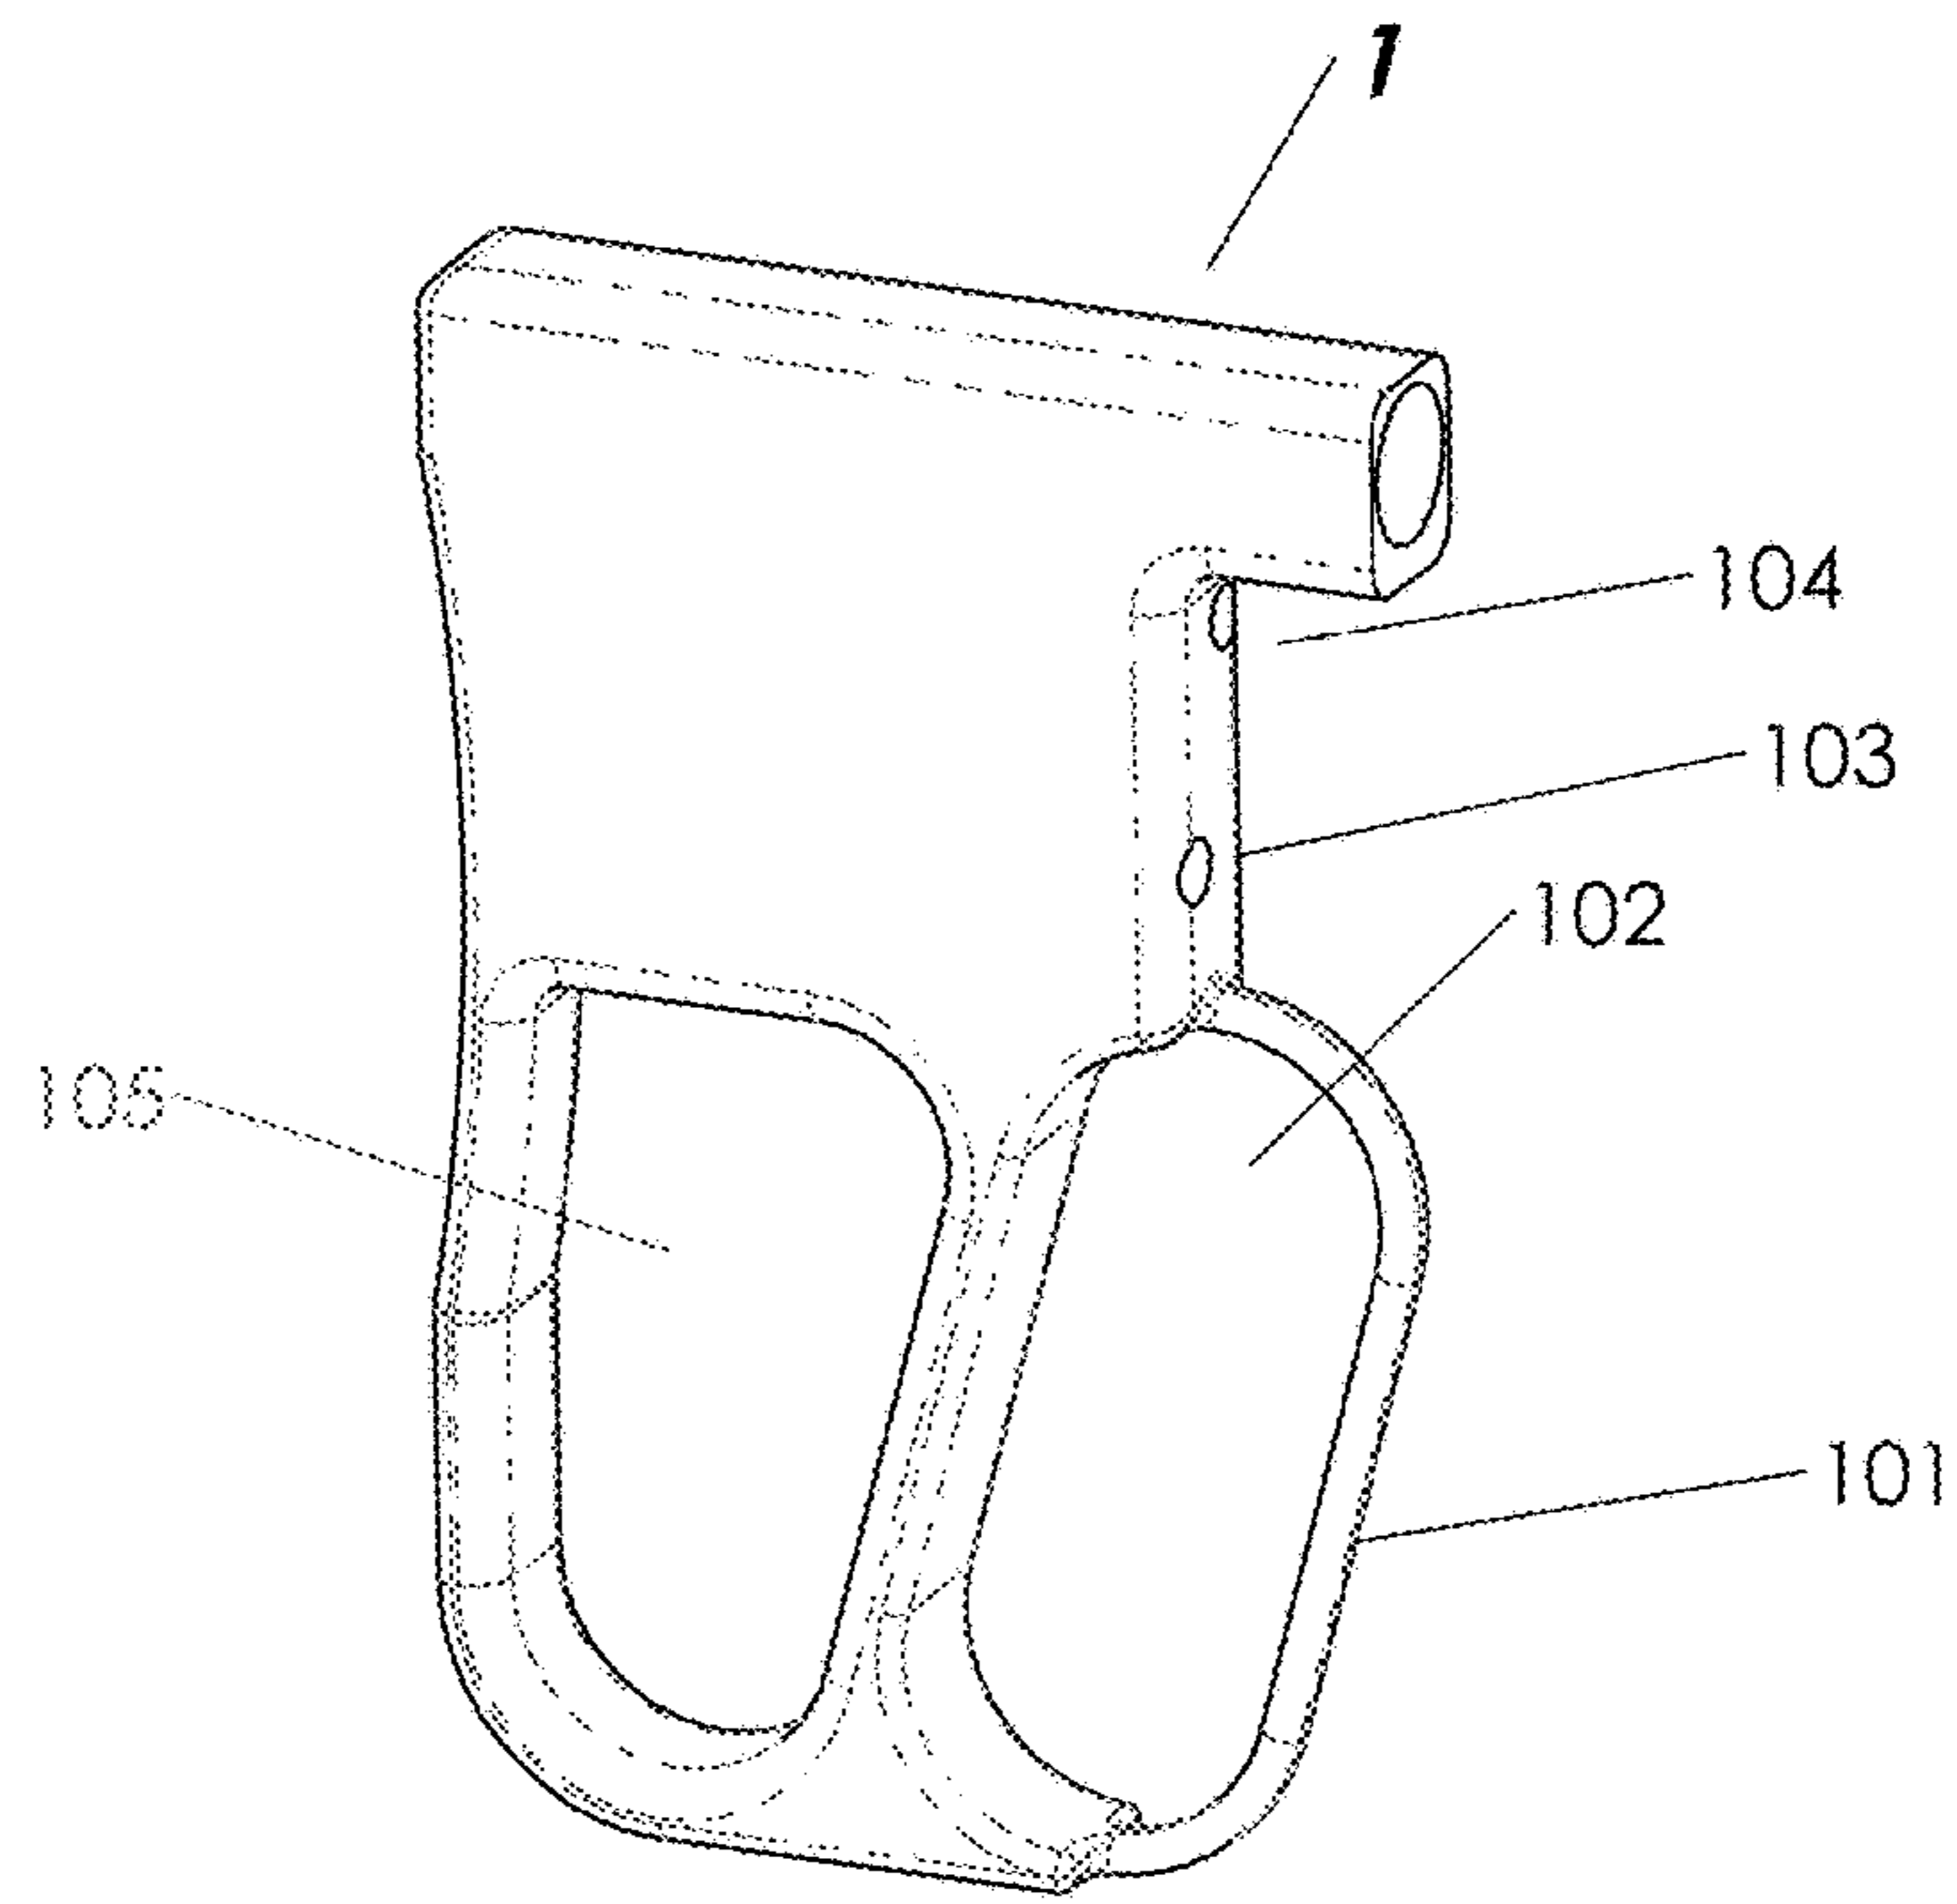


Fig. 8

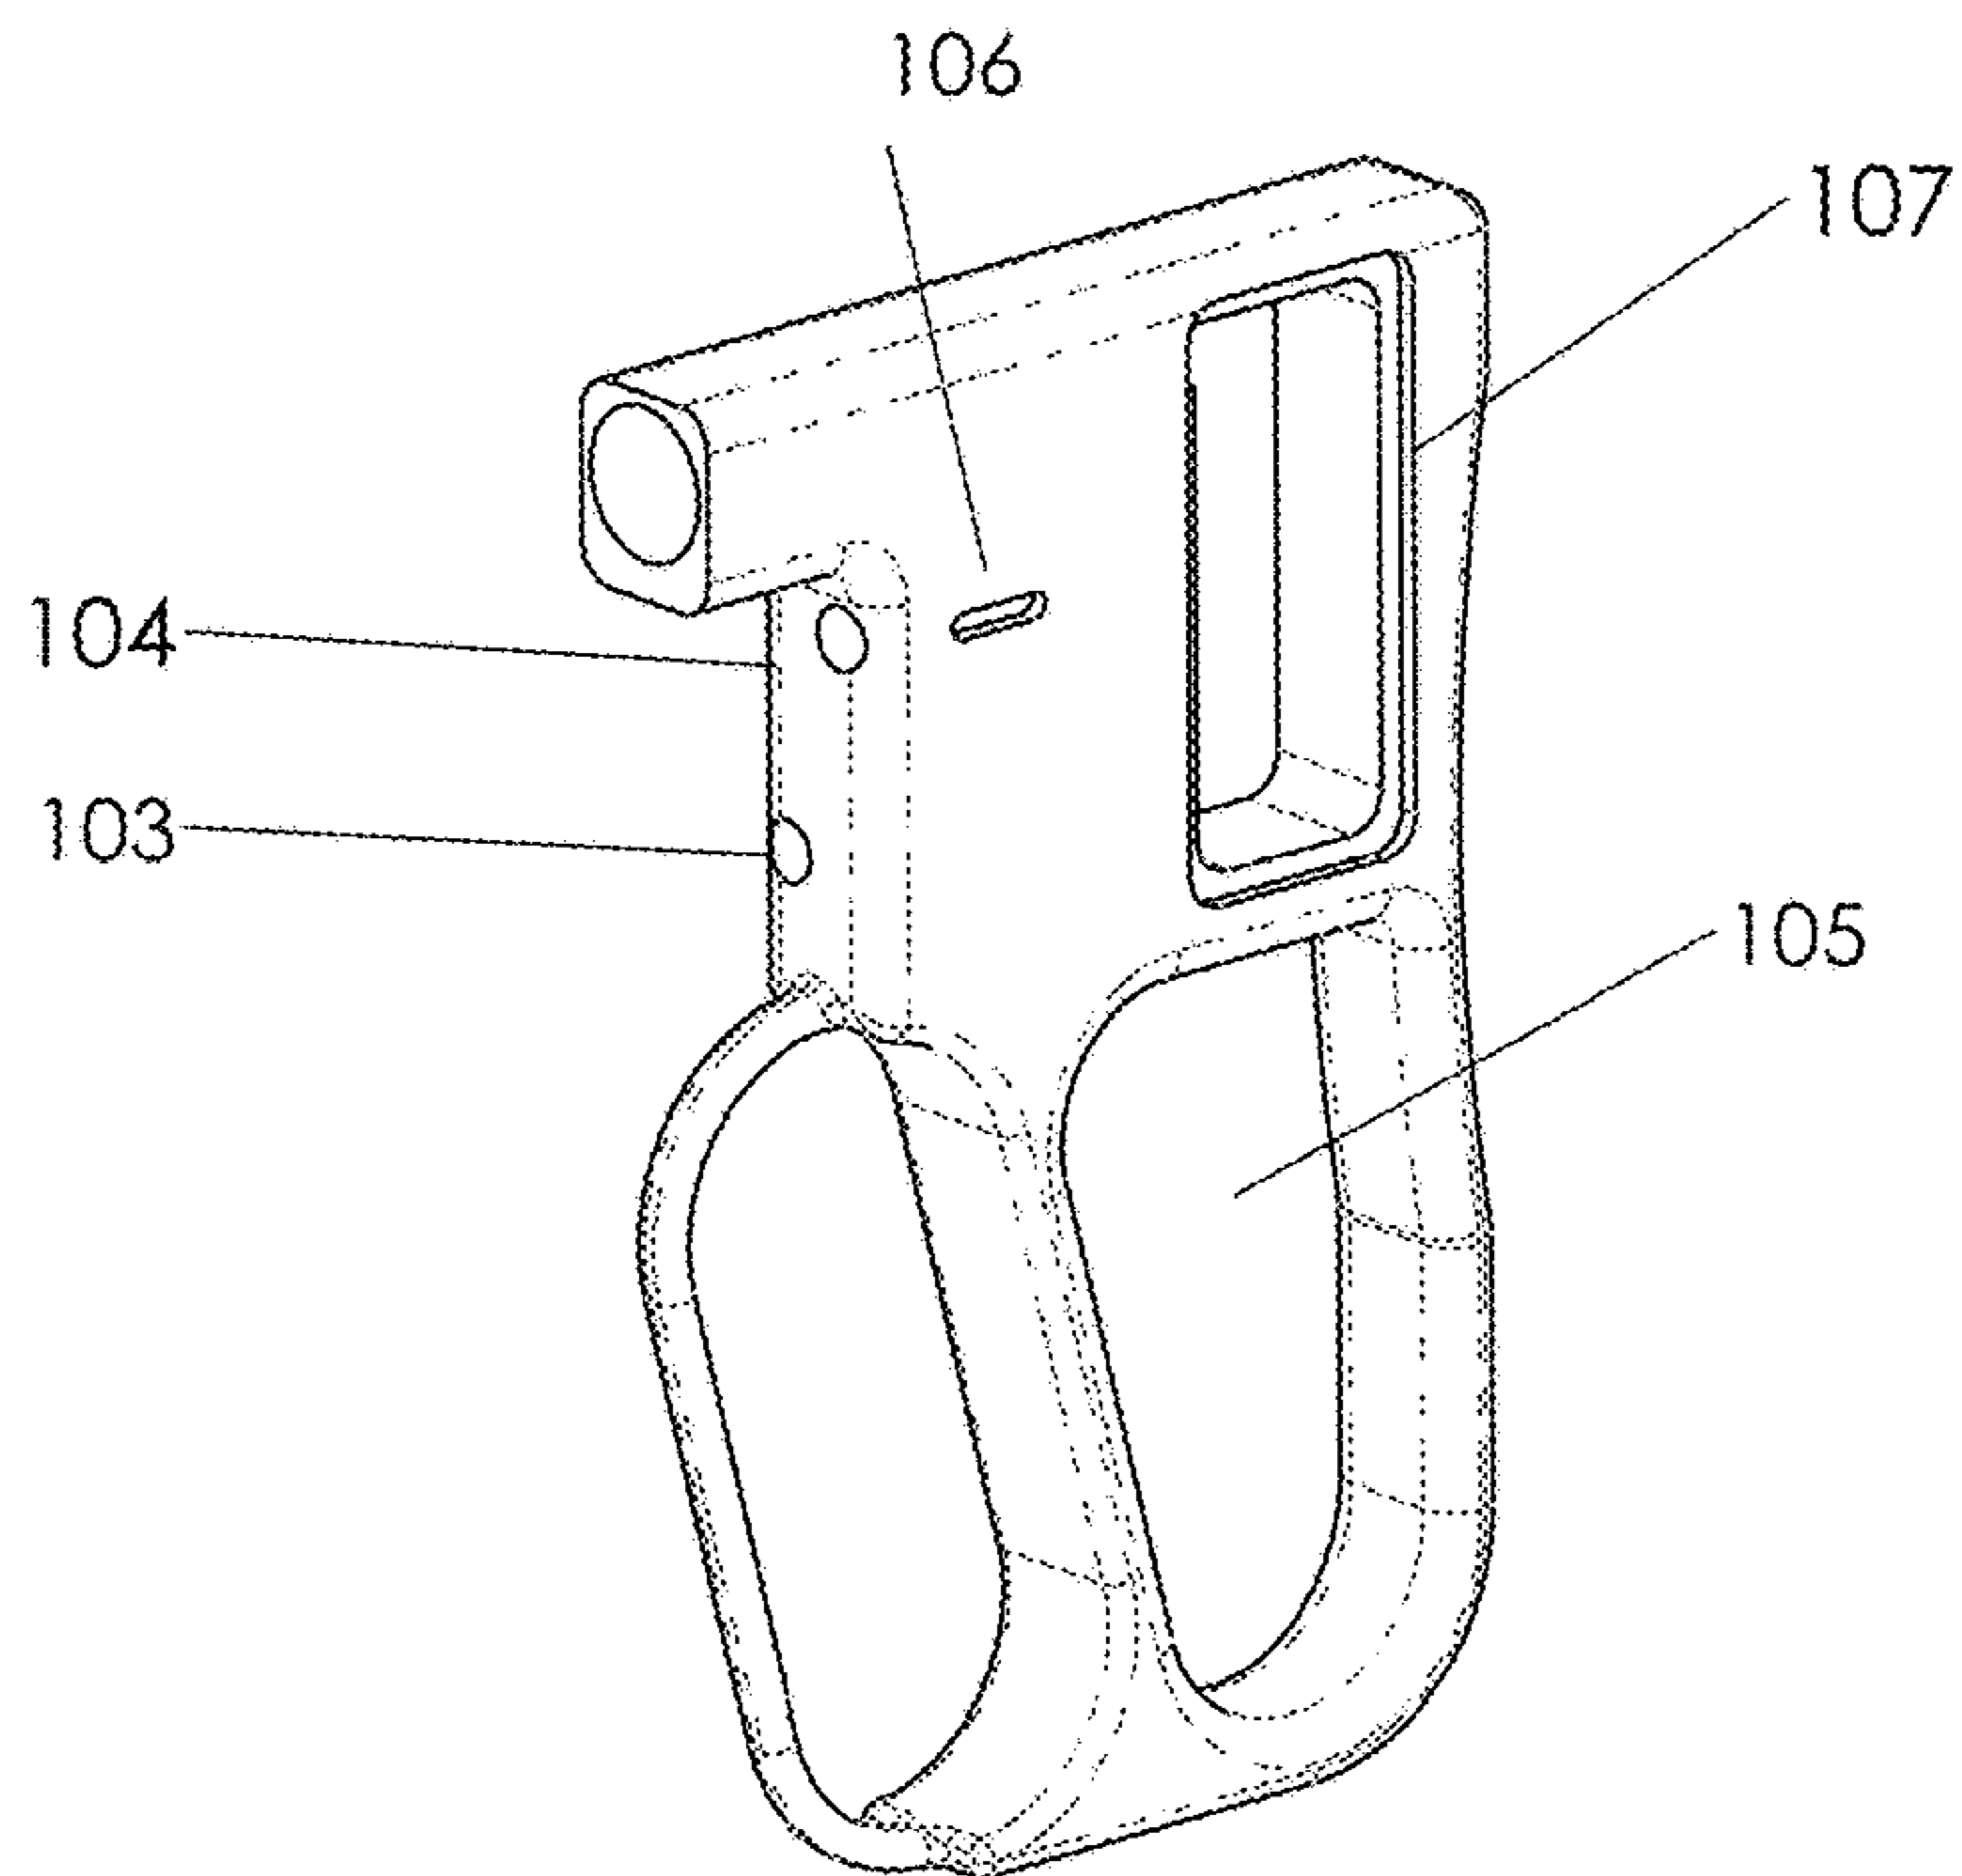


Fig. 9

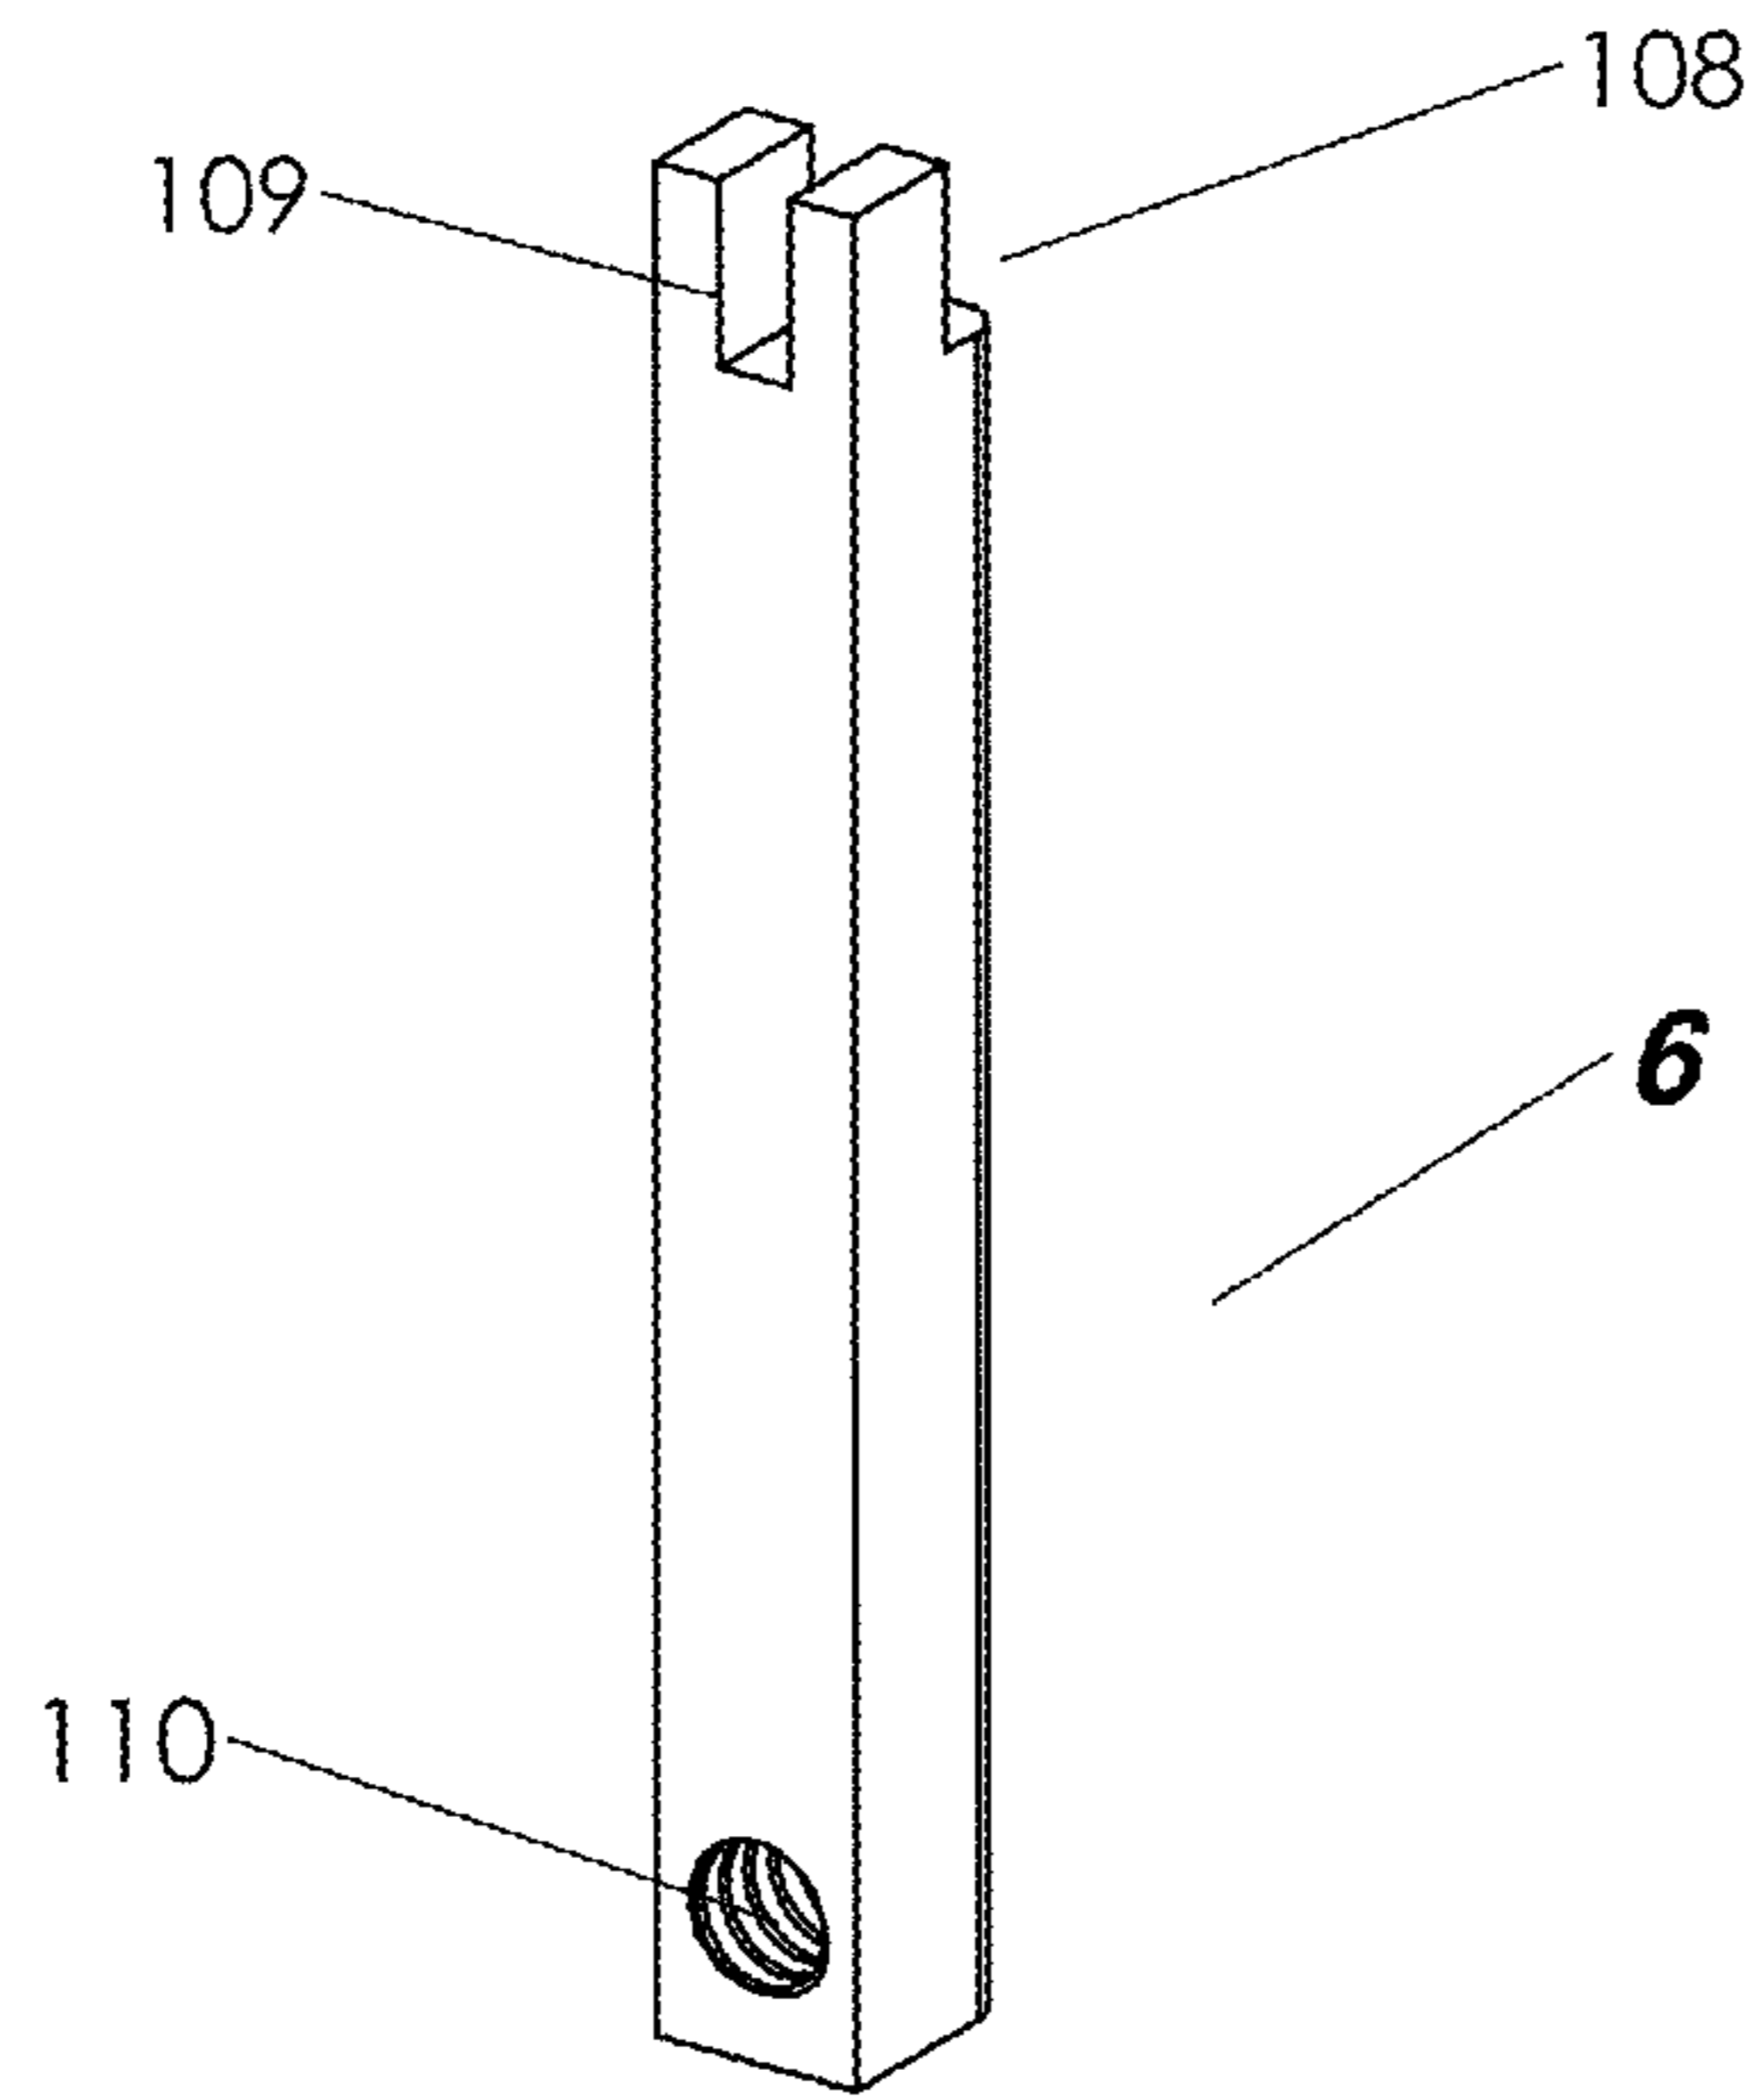


Fig. 10

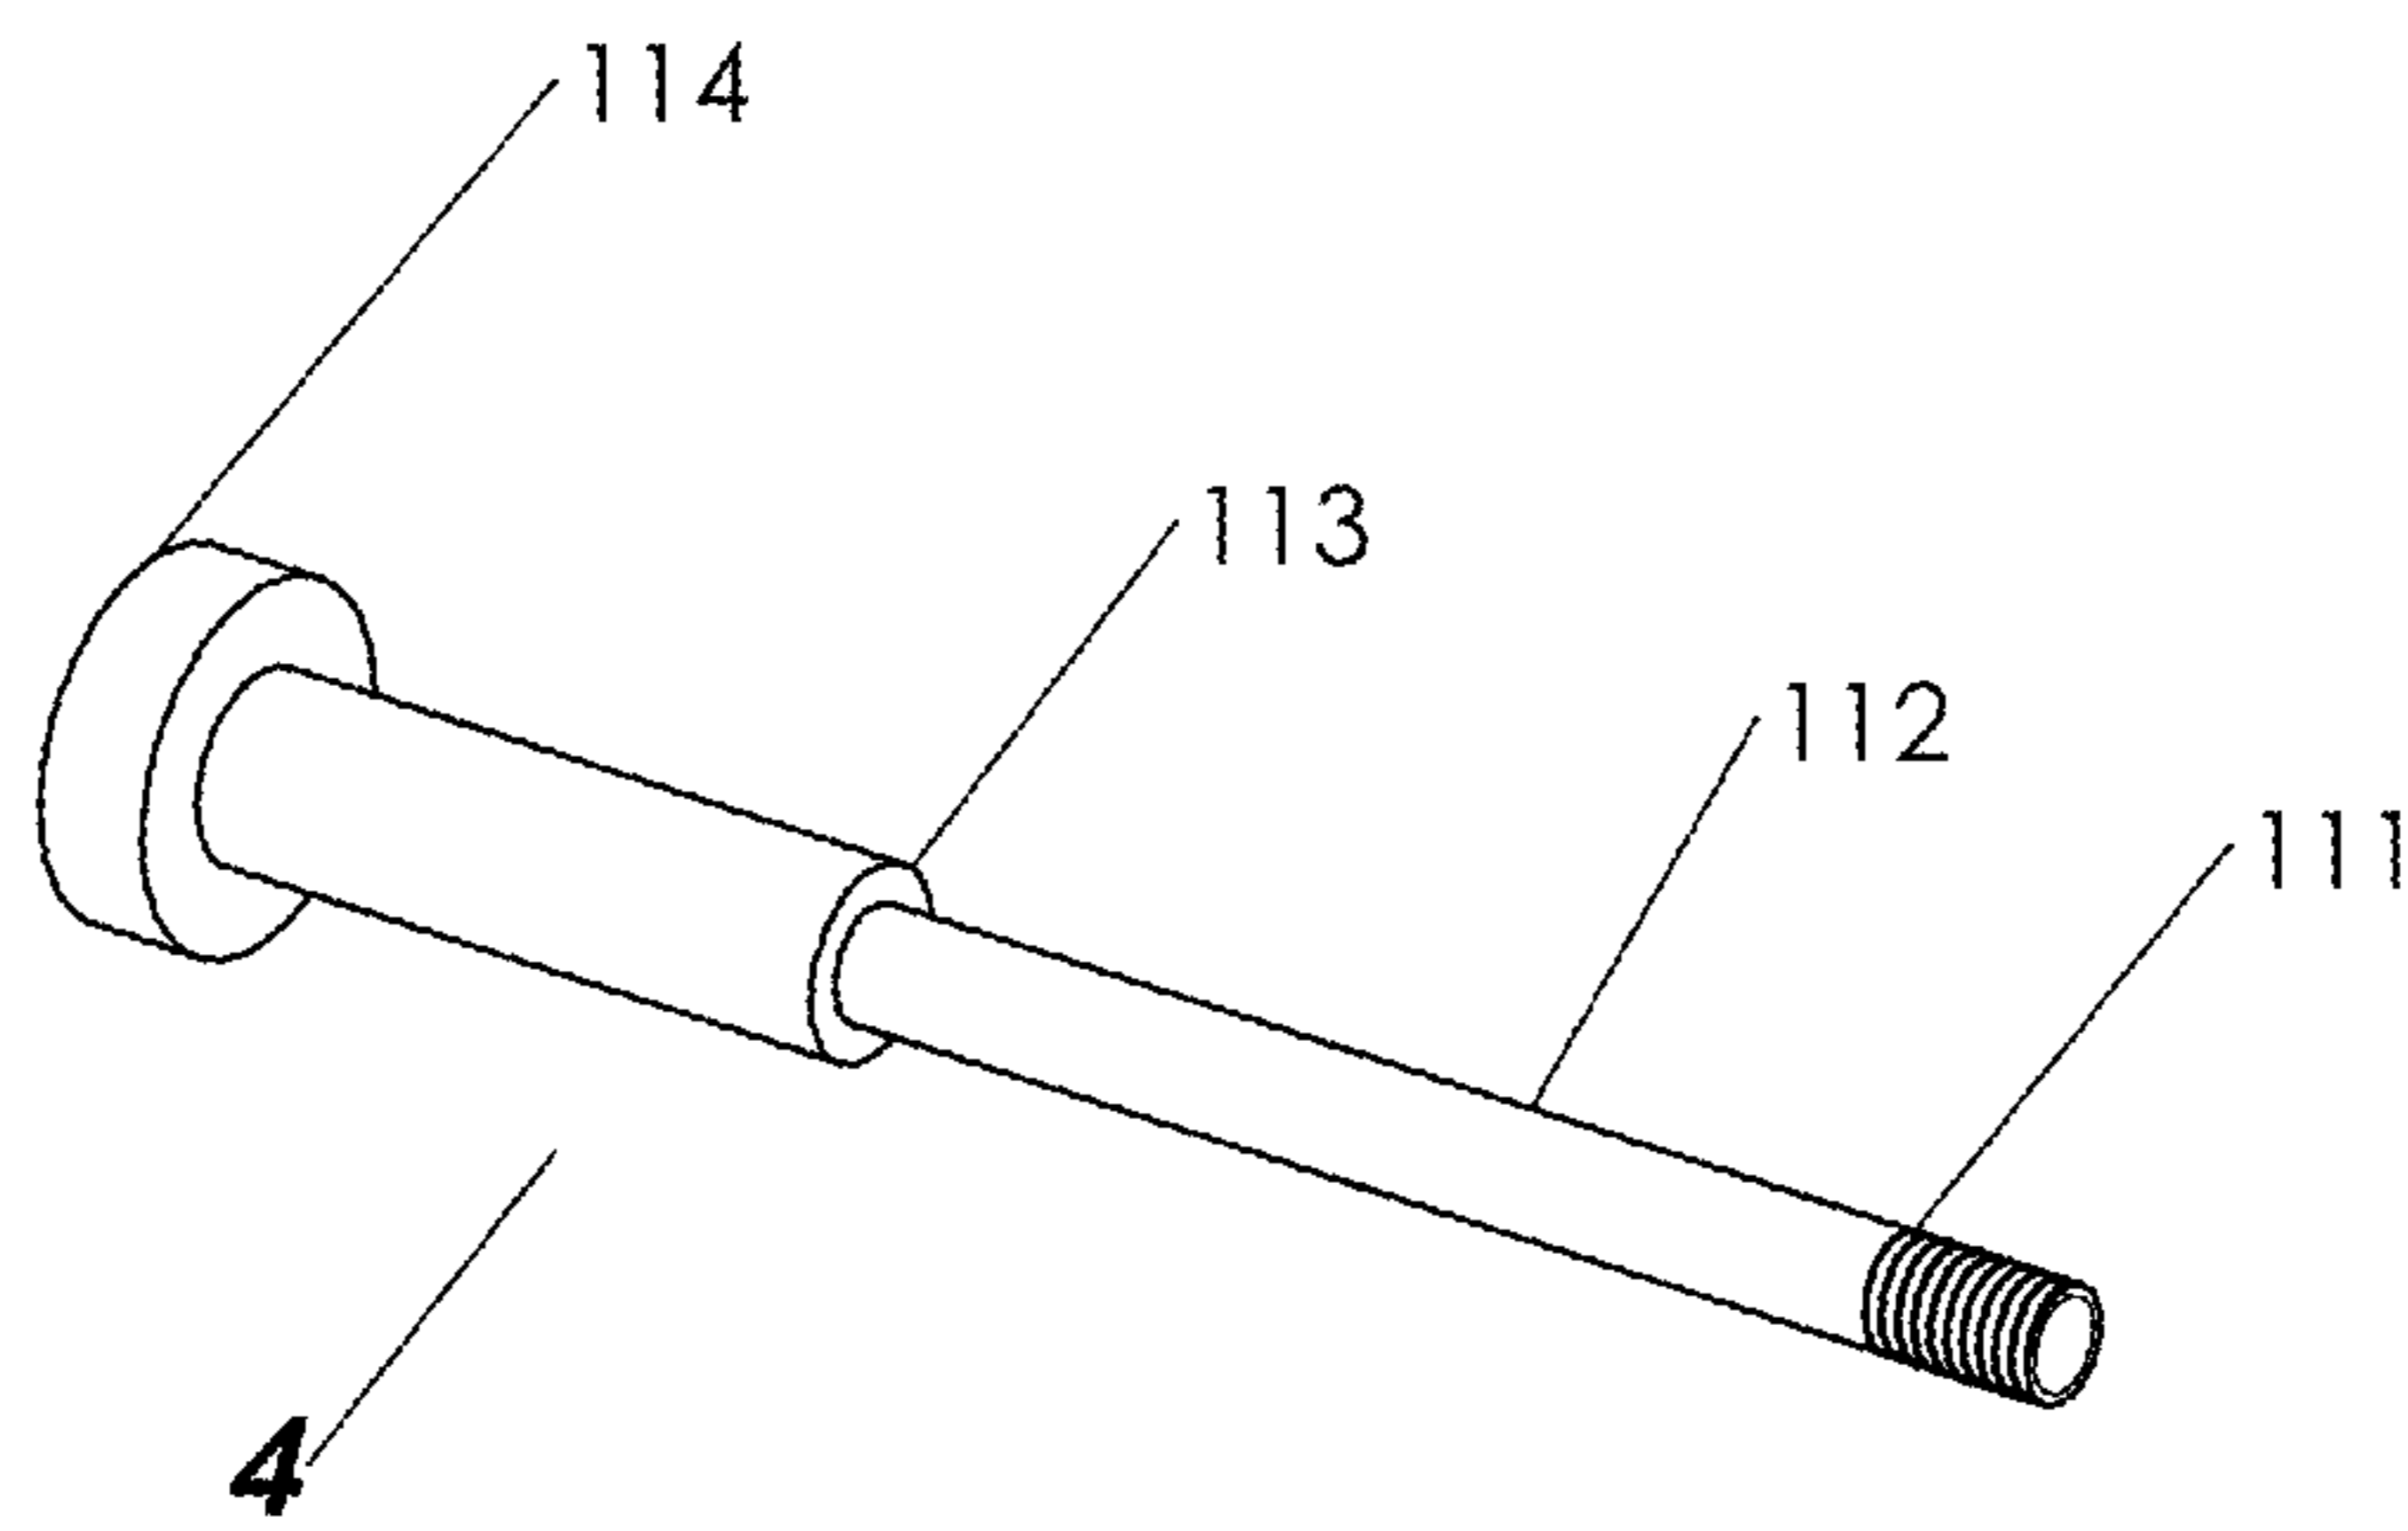


Fig. 11

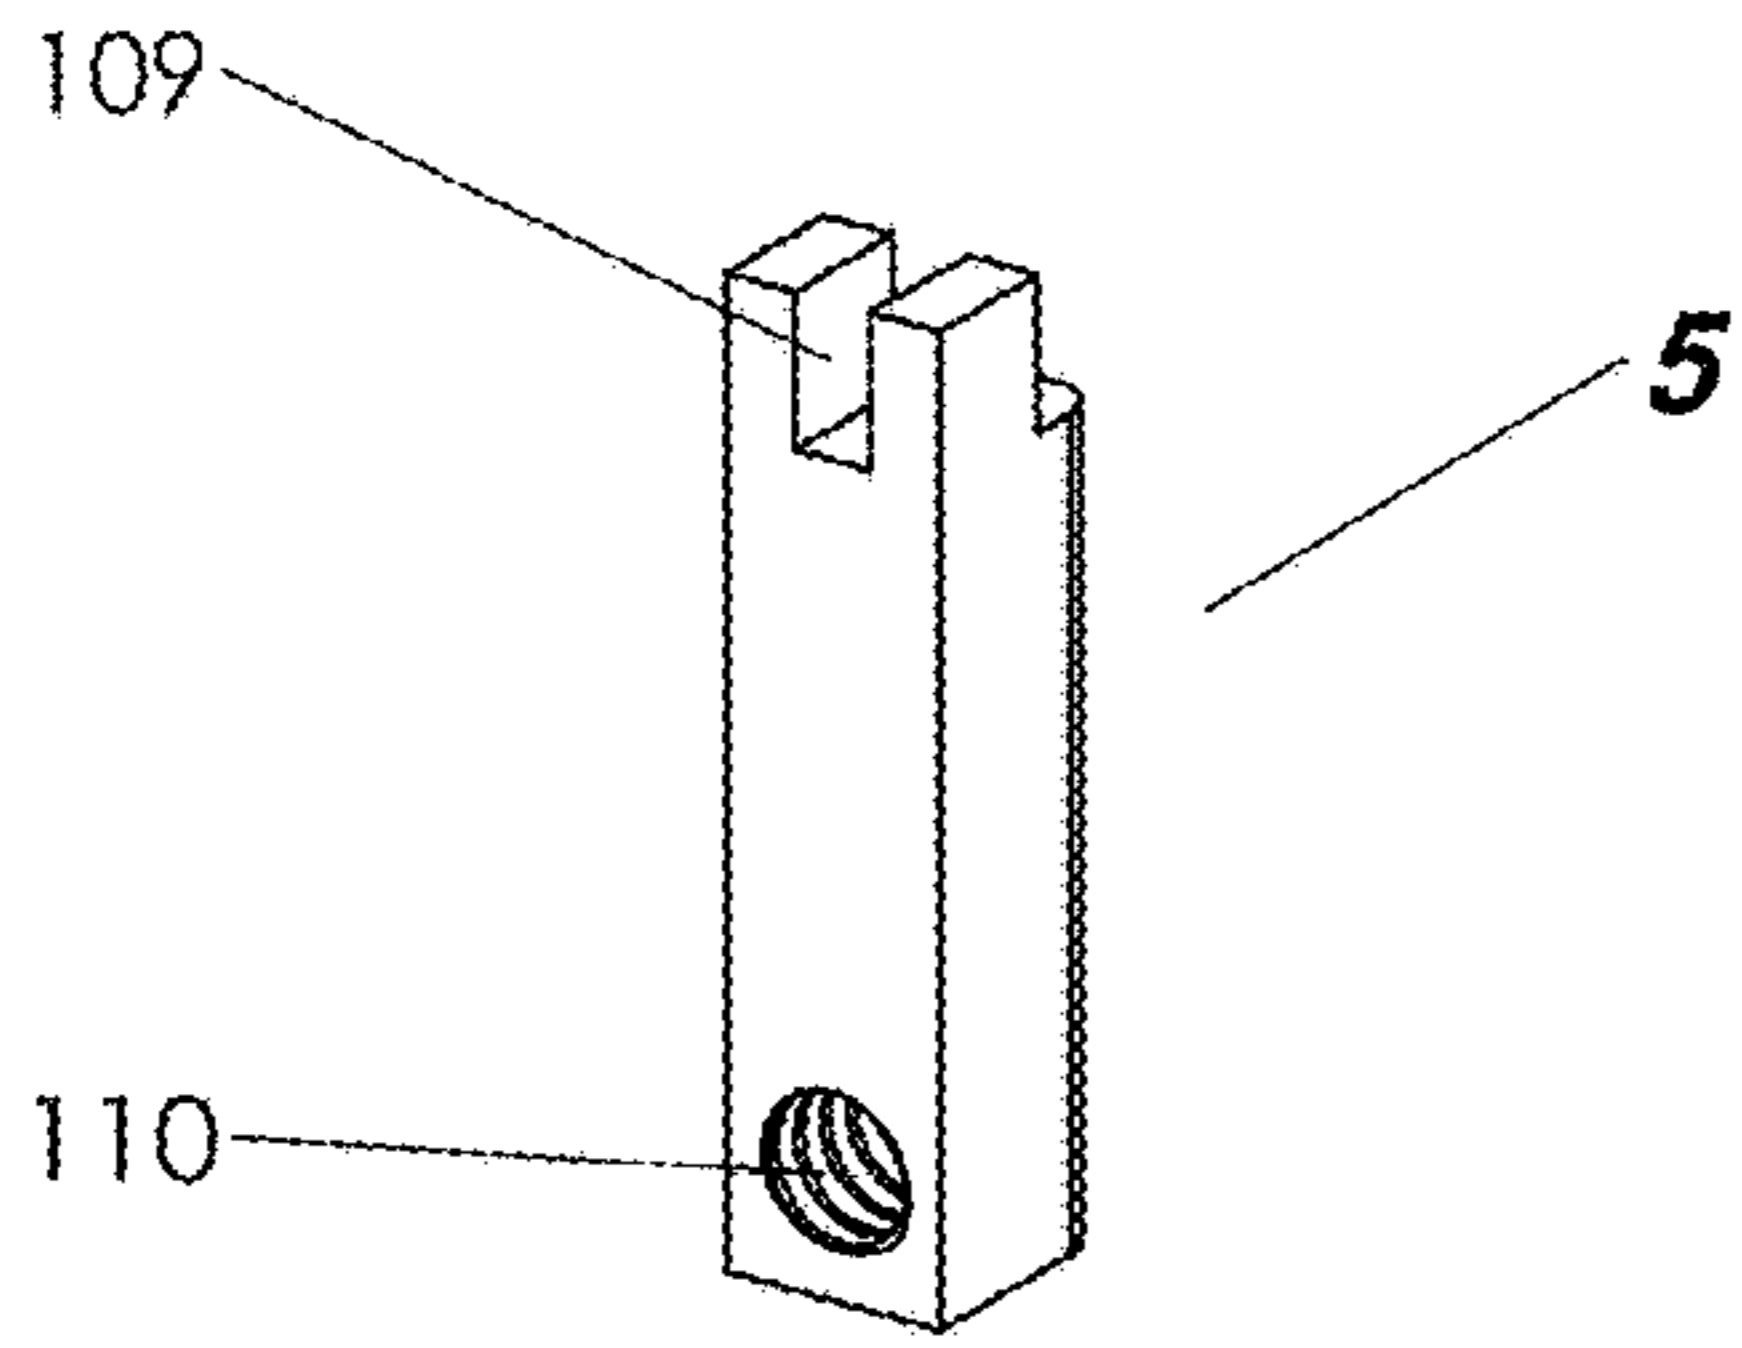


Fig. 12

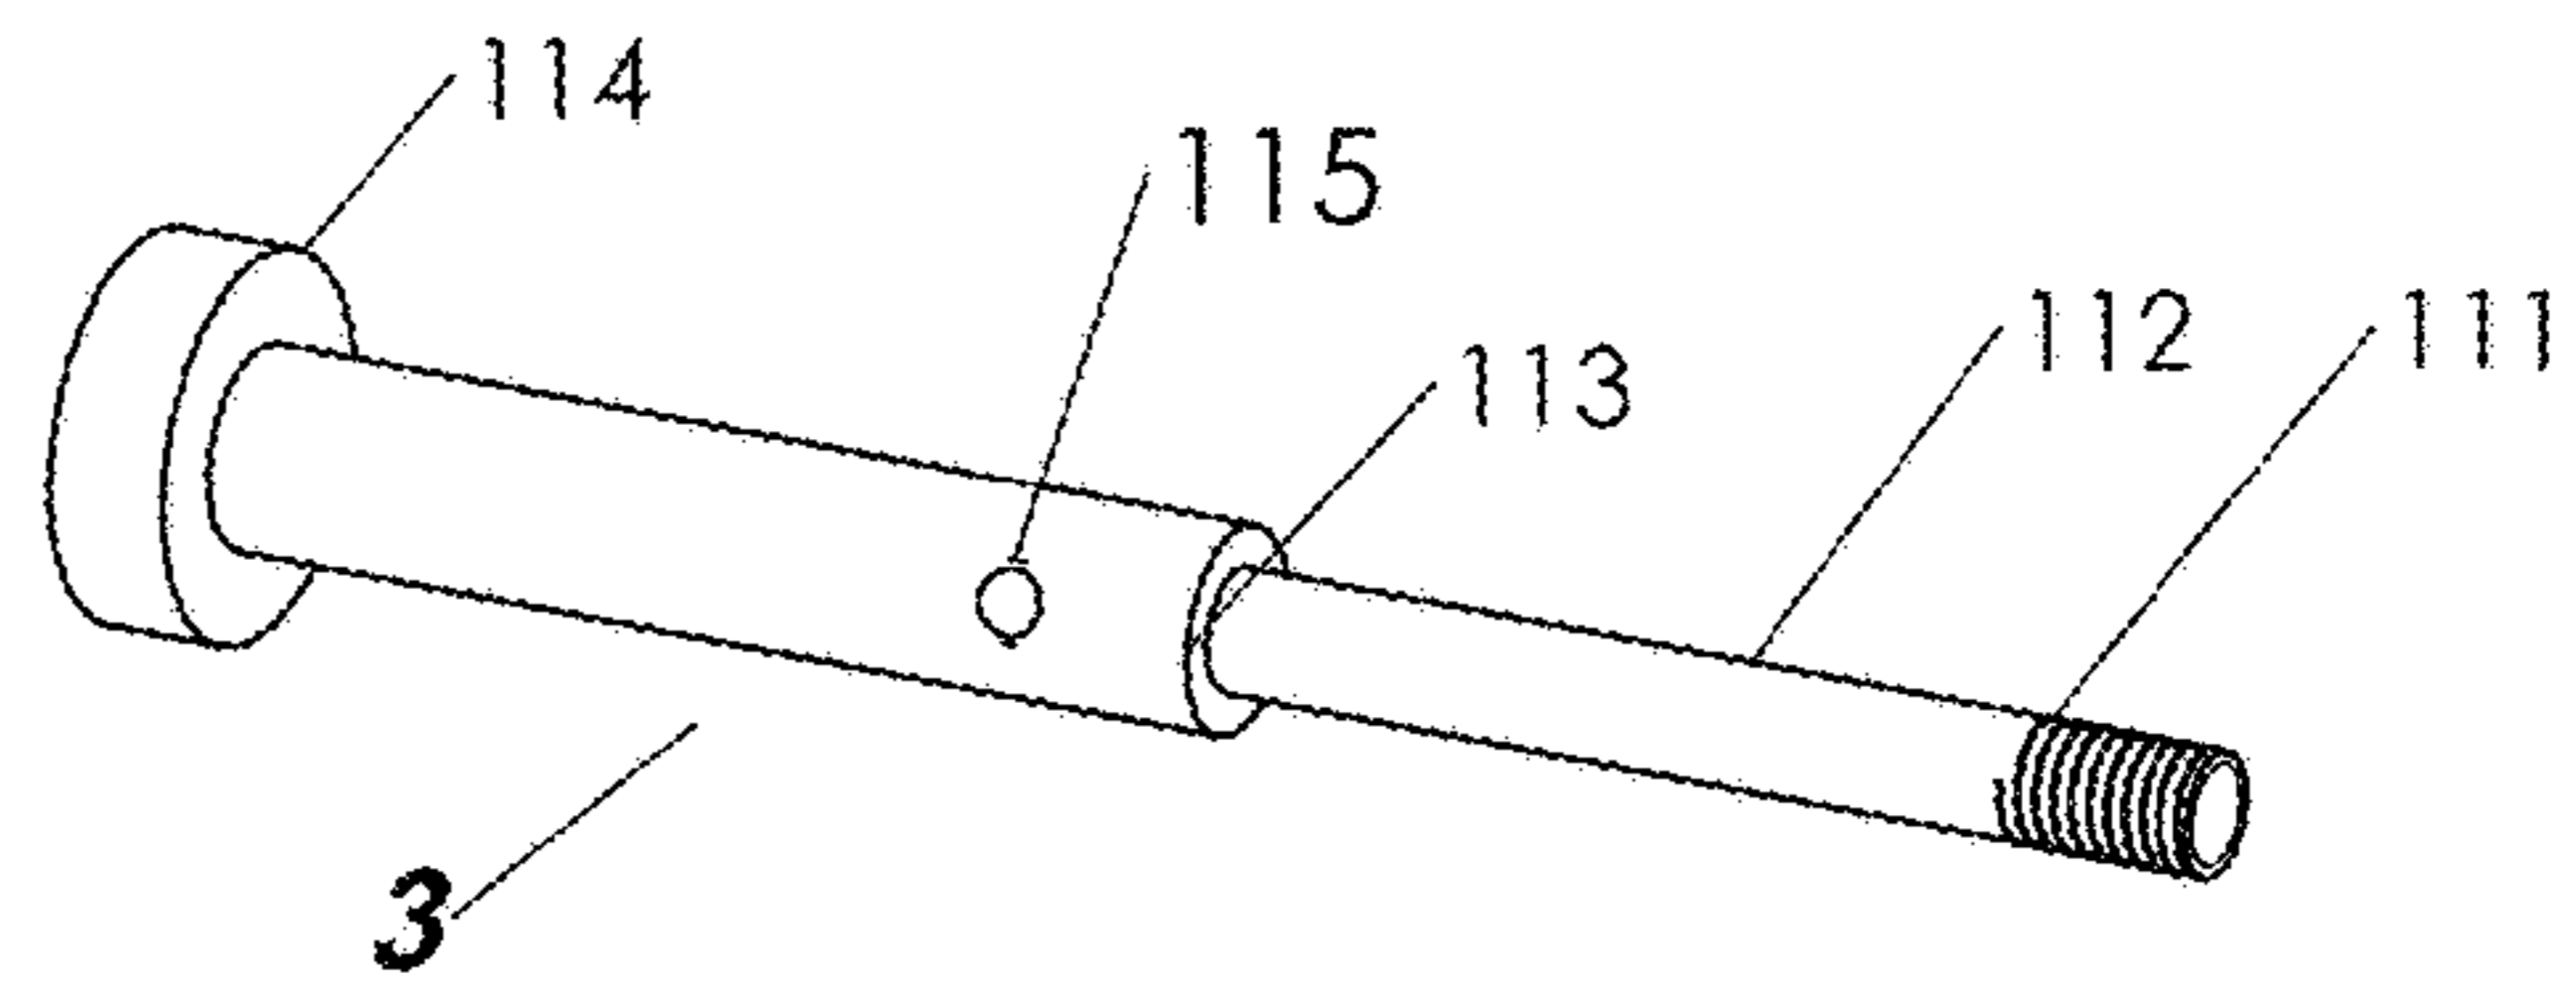


Fig. 13

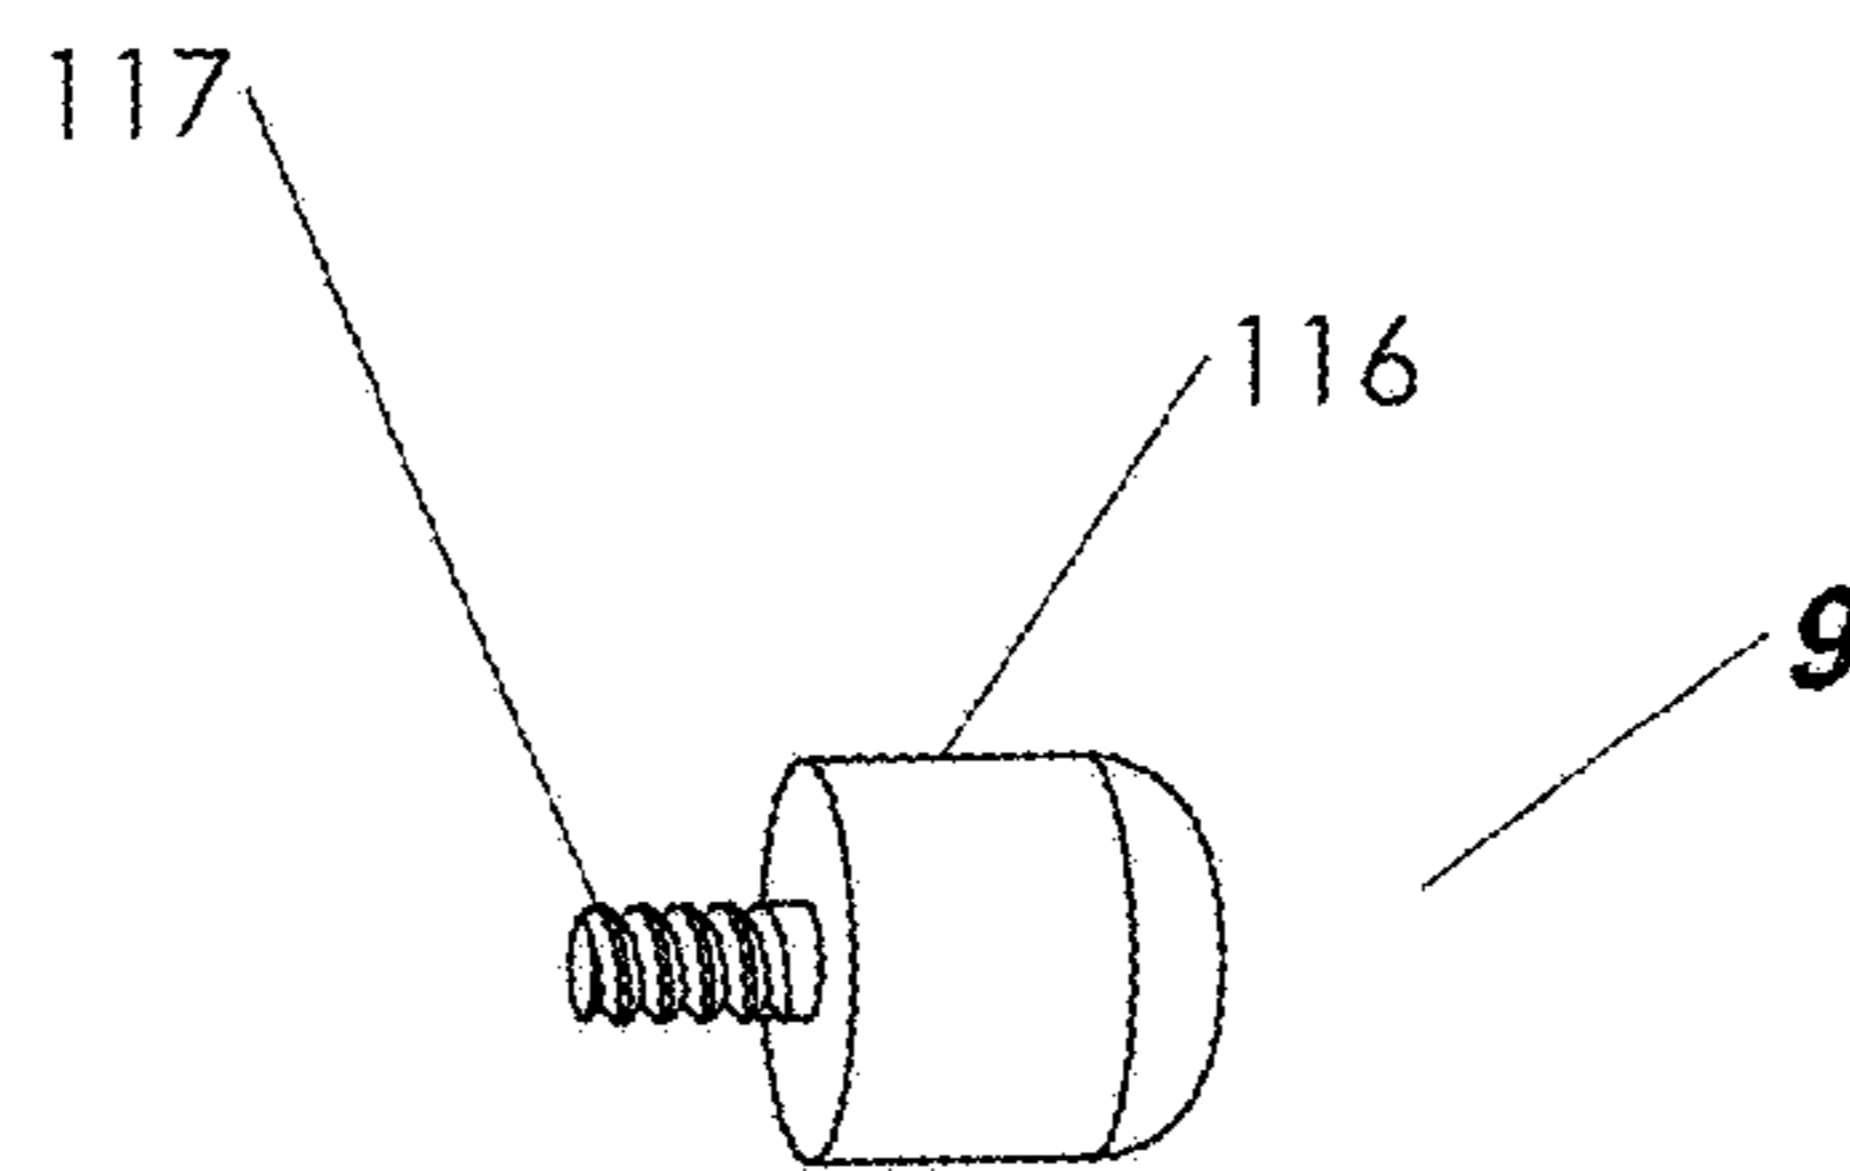


Fig. 14

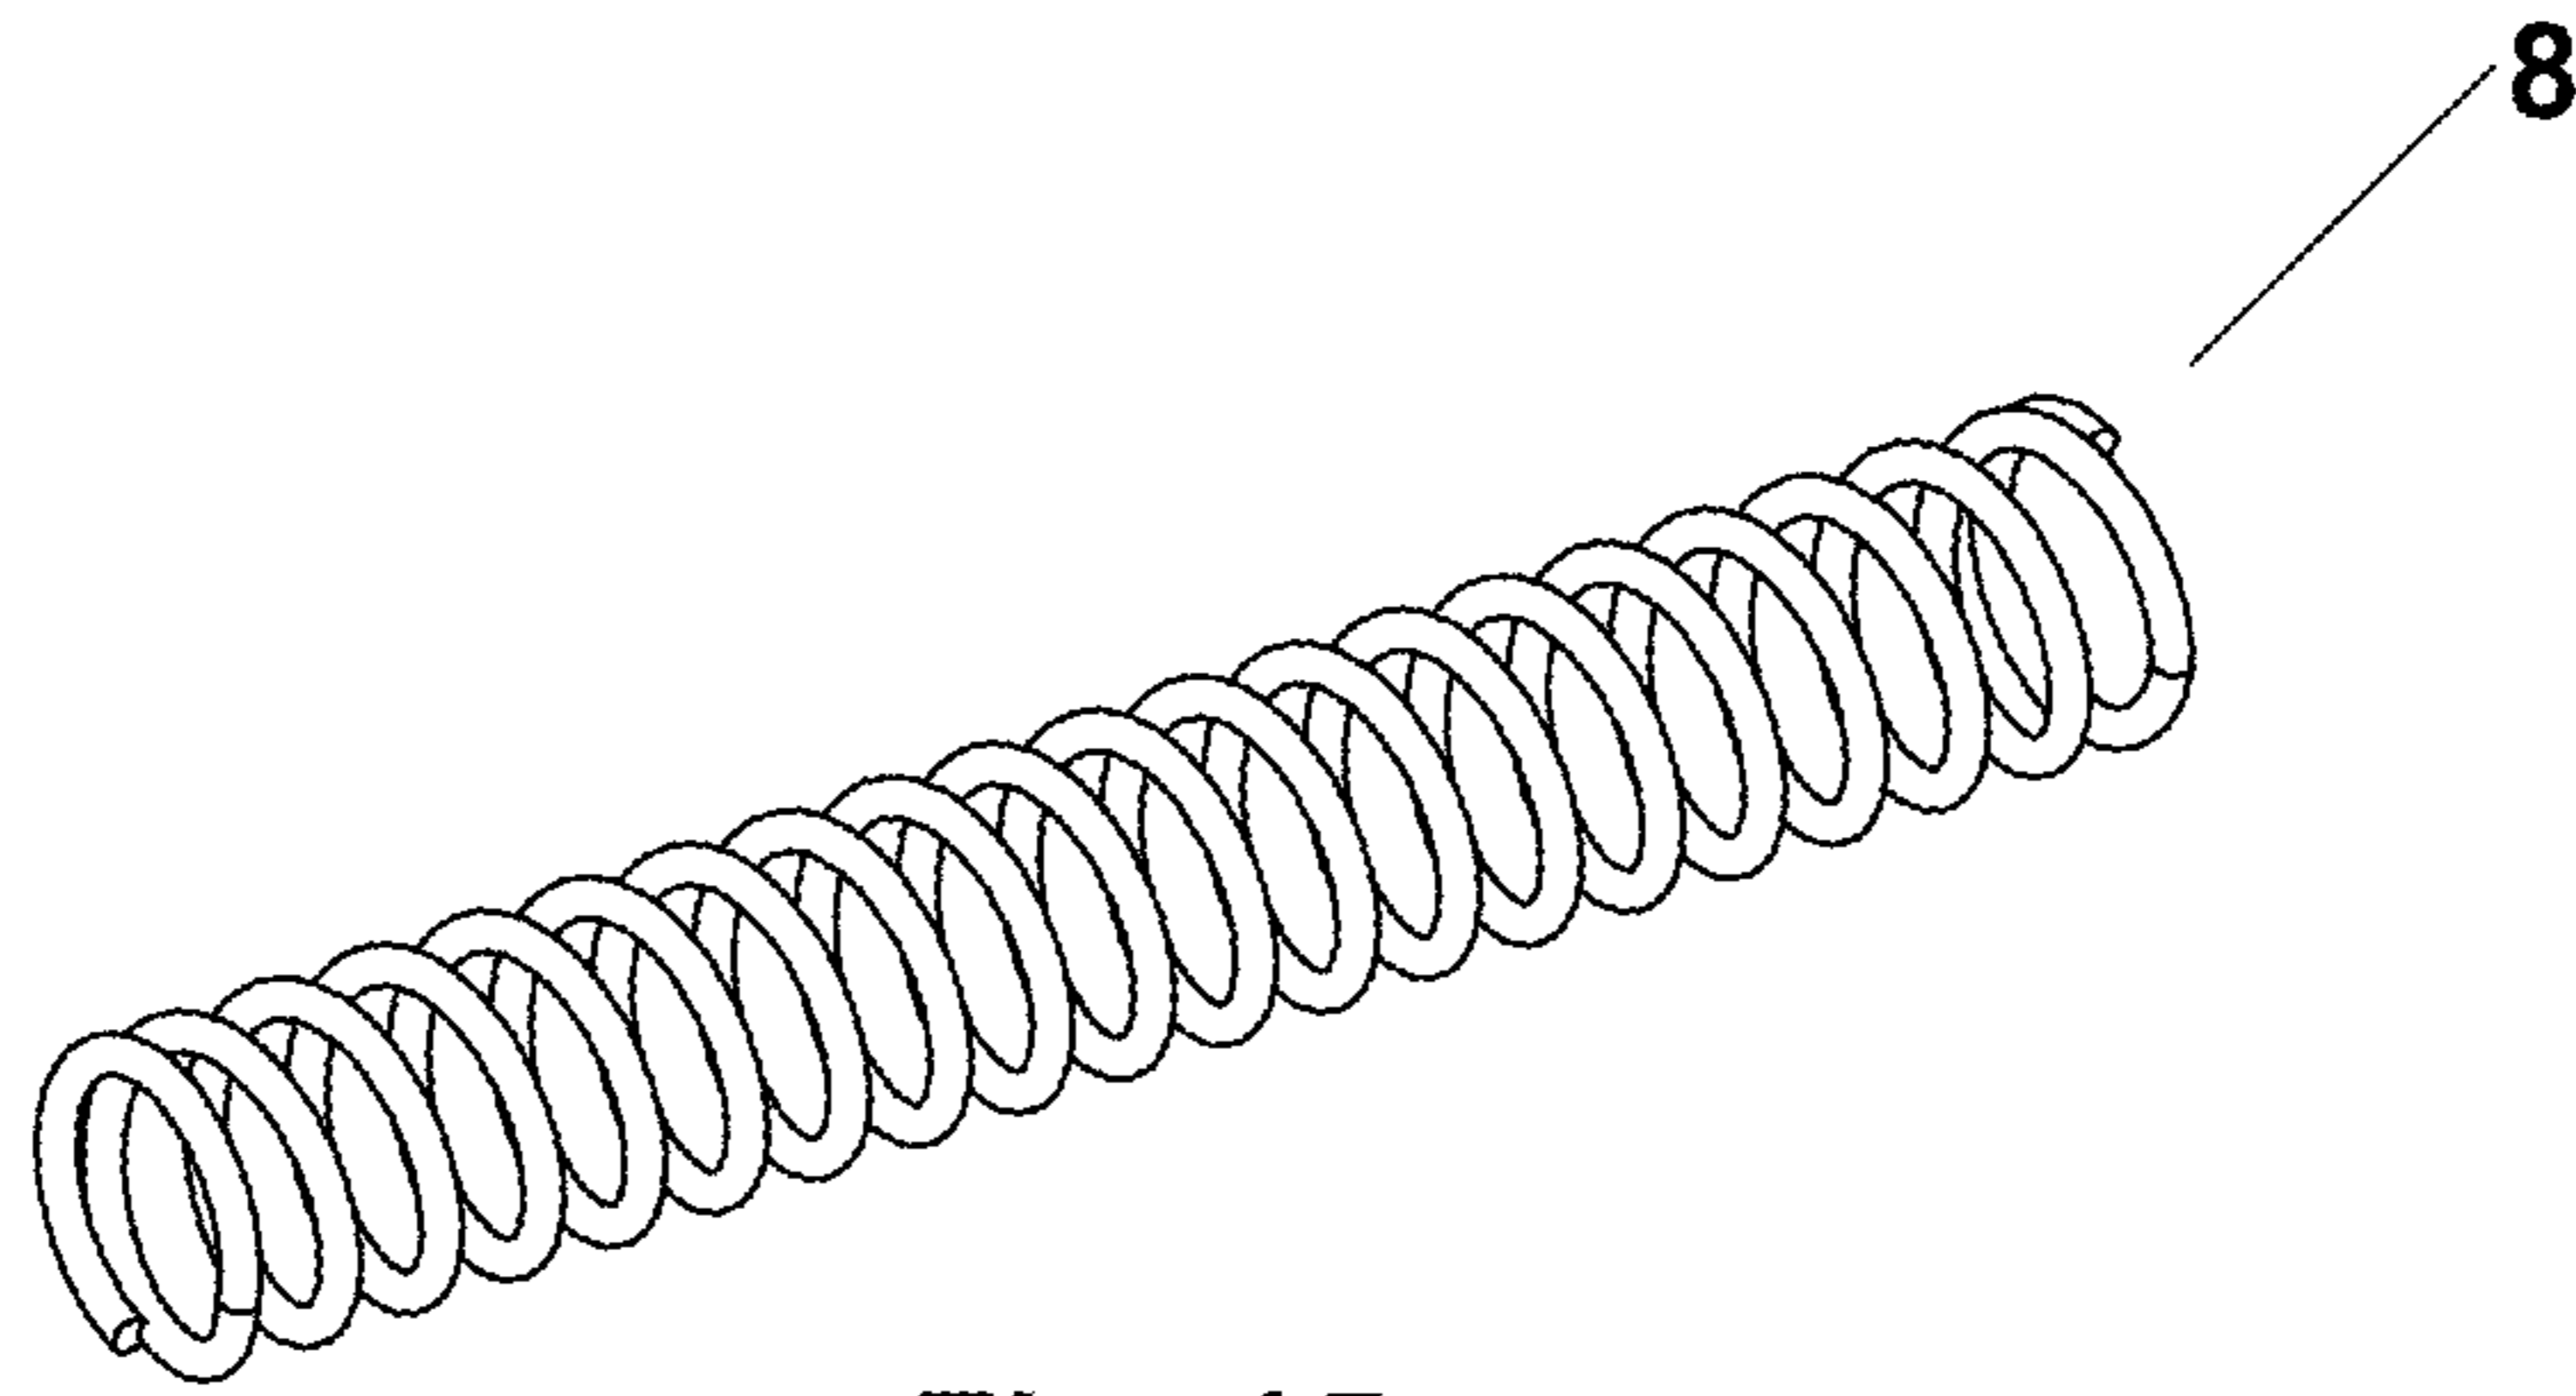


Fig. 15

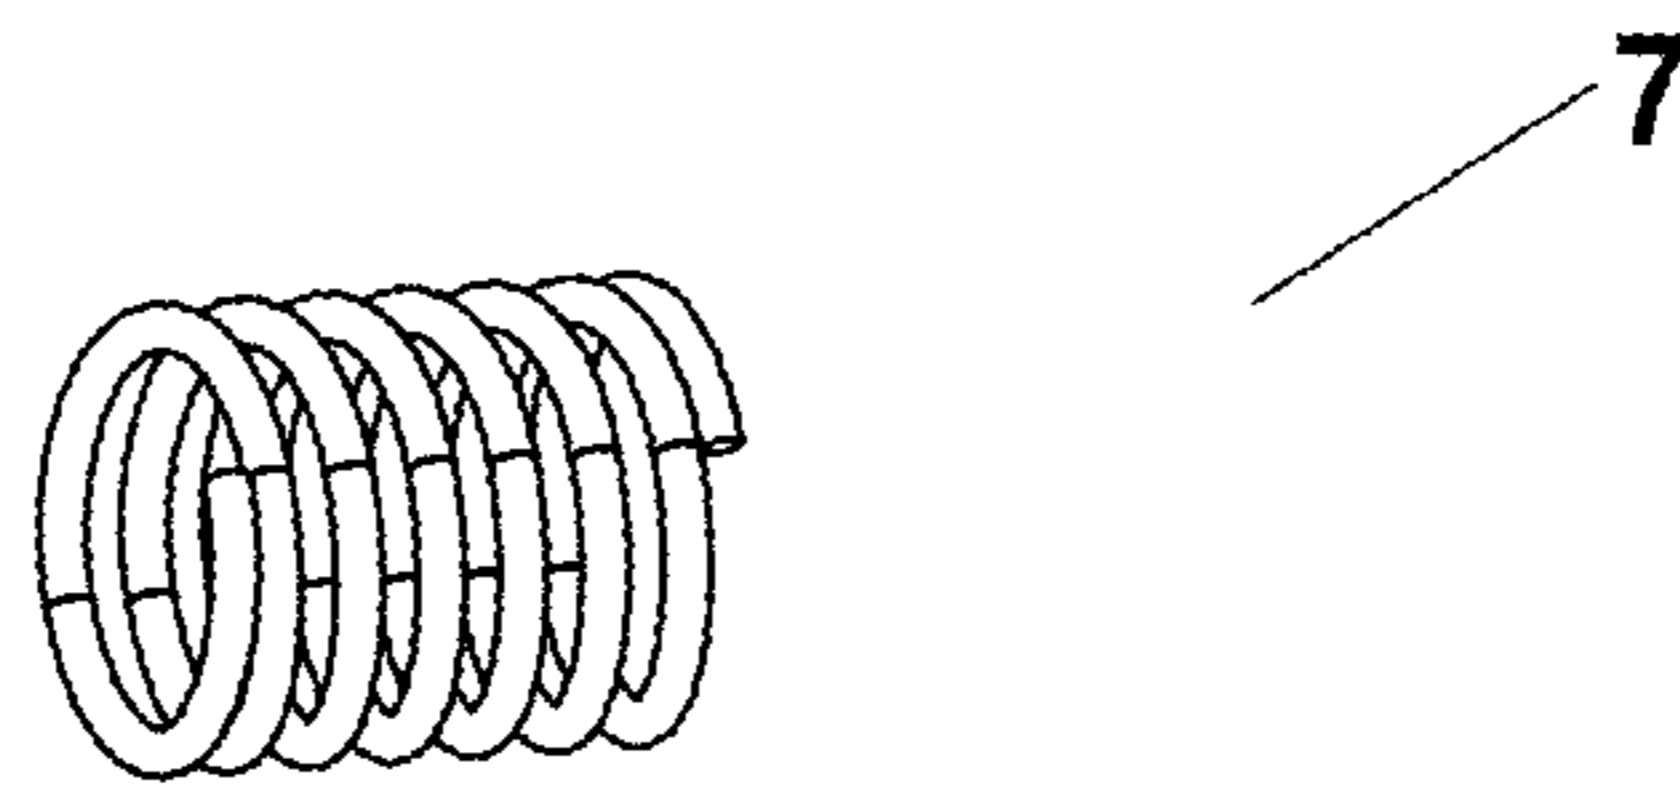


Fig. 16

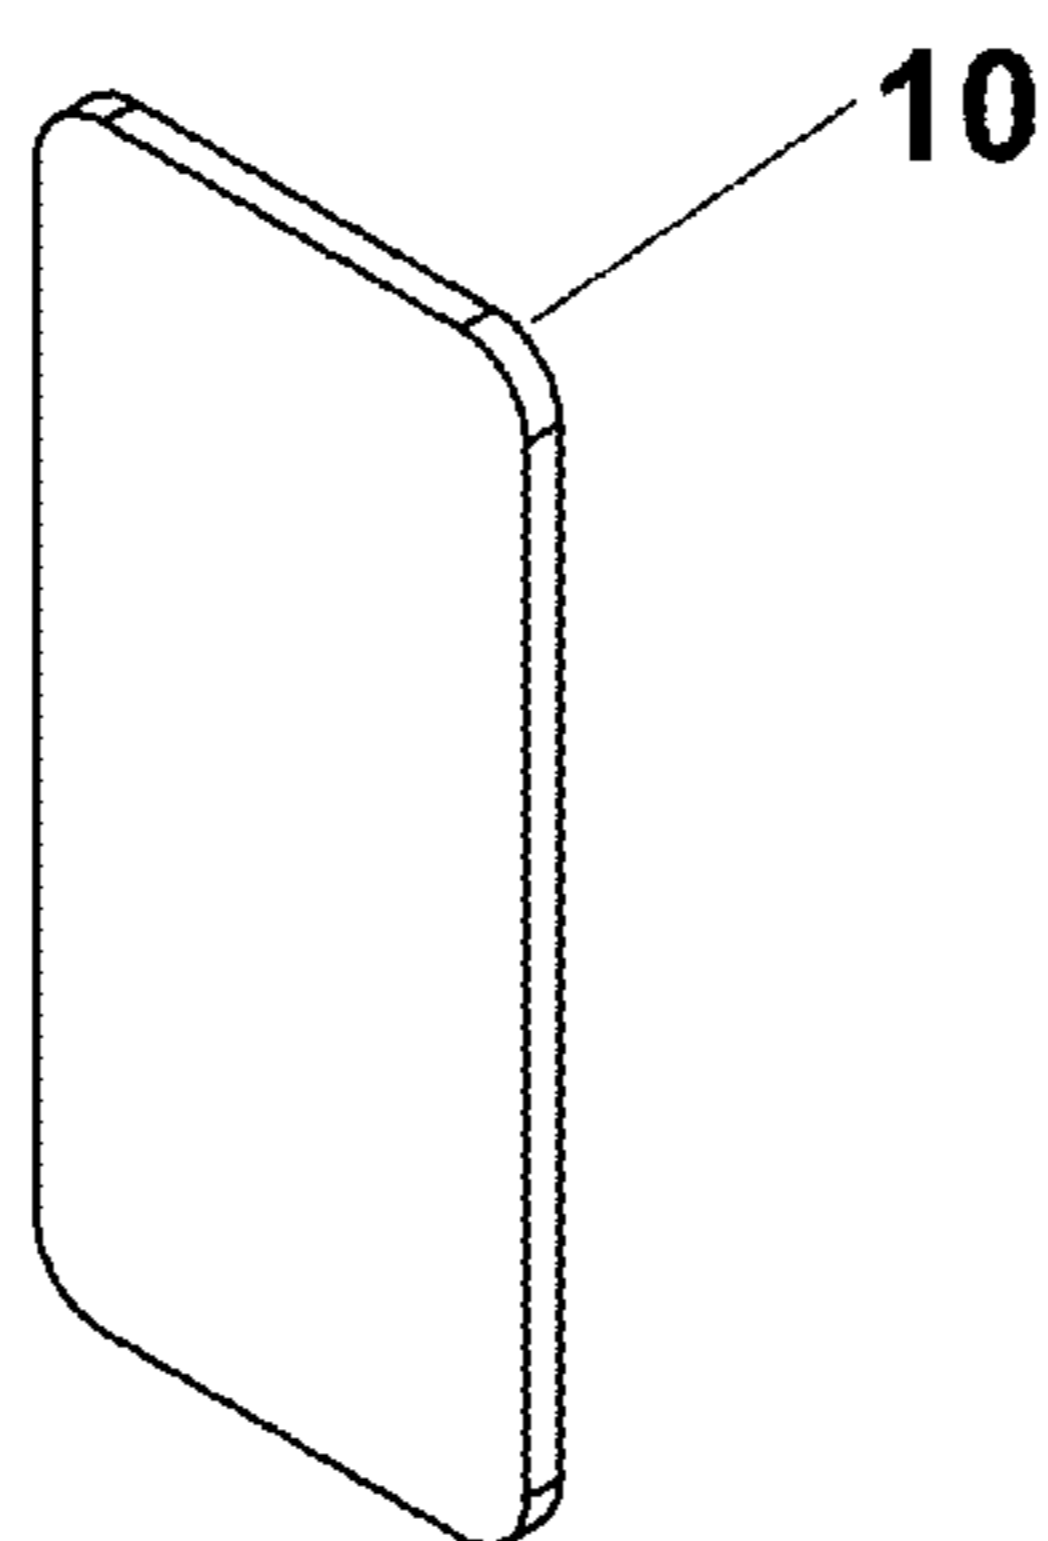


Fig. 17

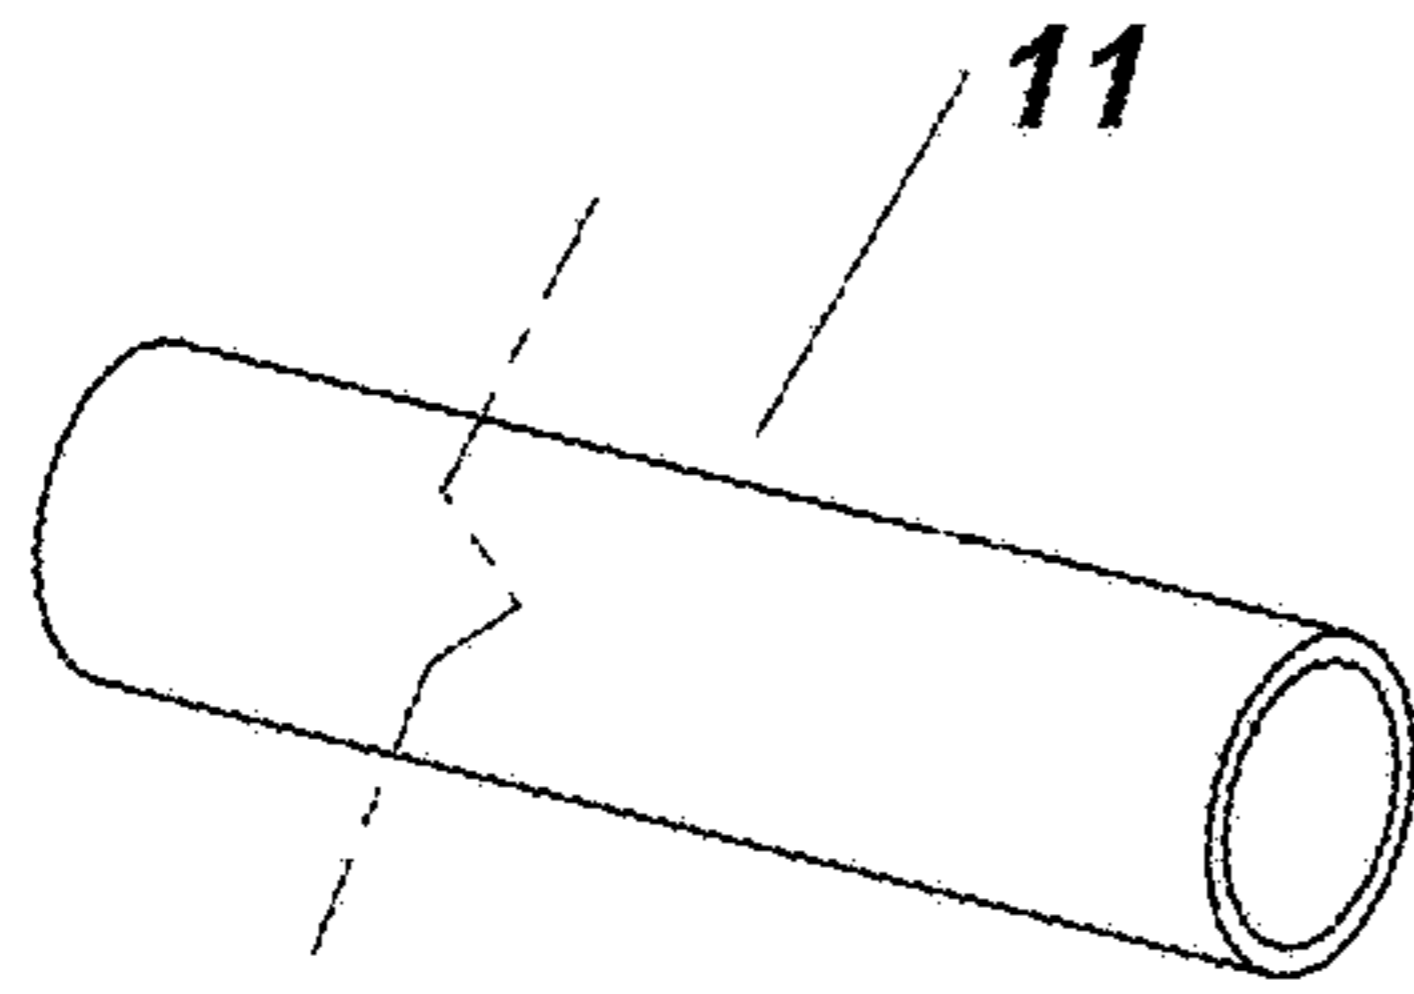


Fig. 18

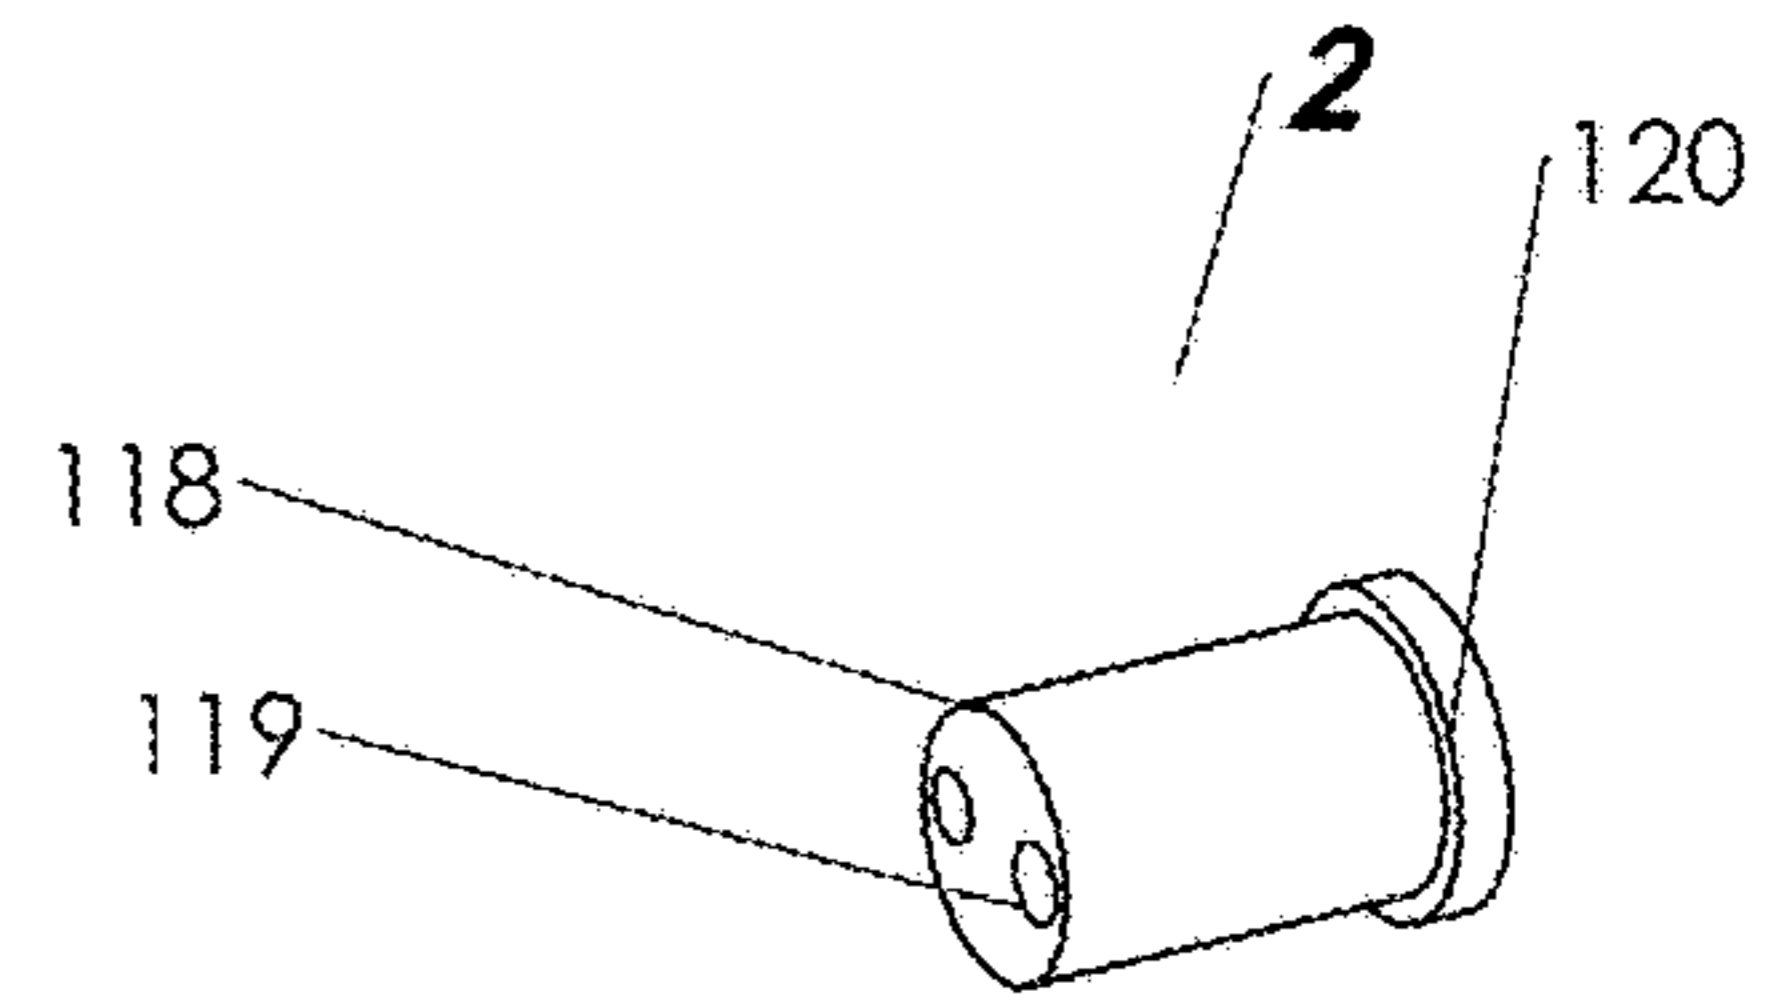


Fig. 19

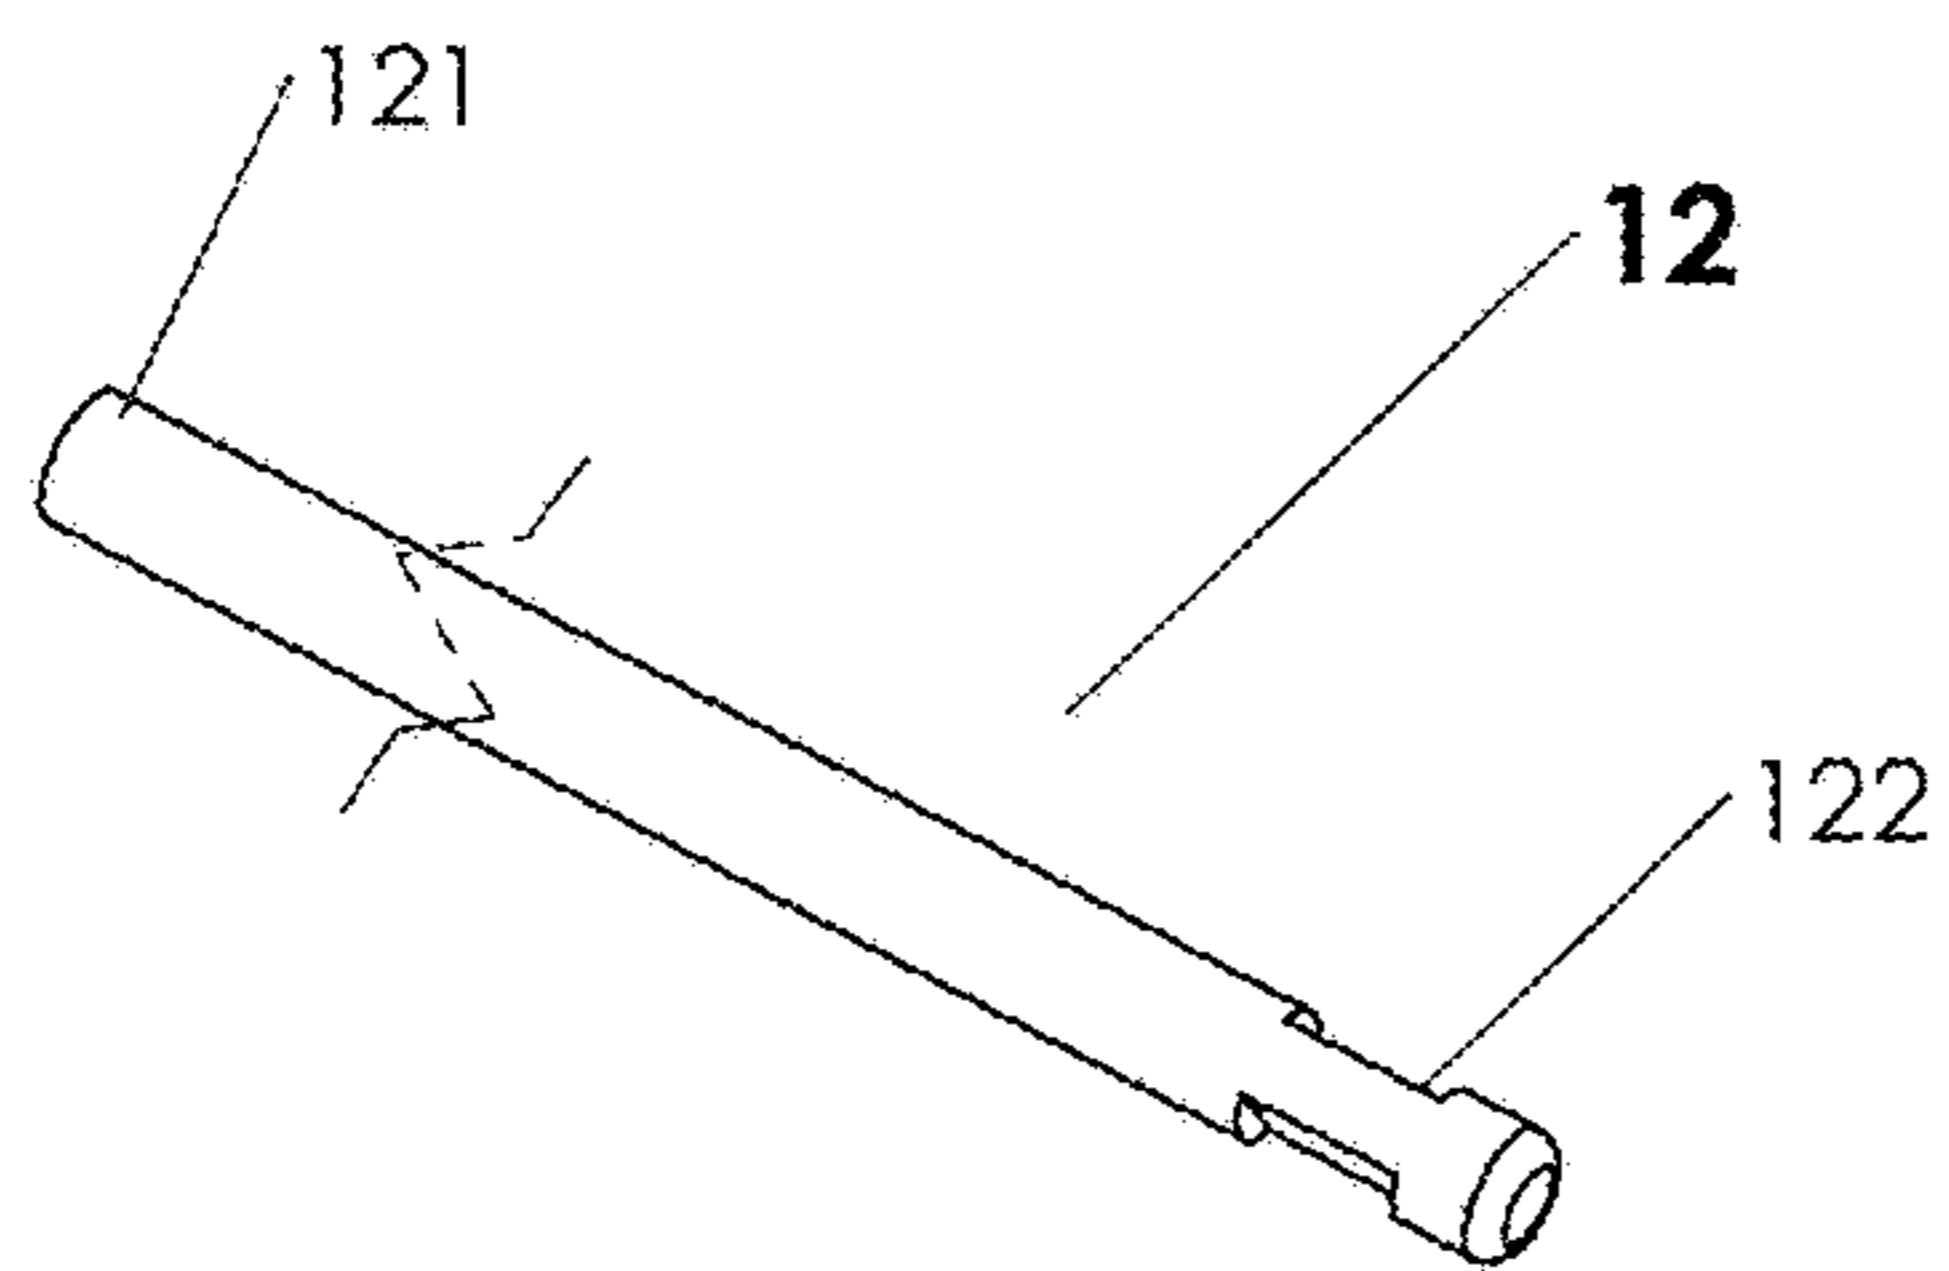


Fig. 20

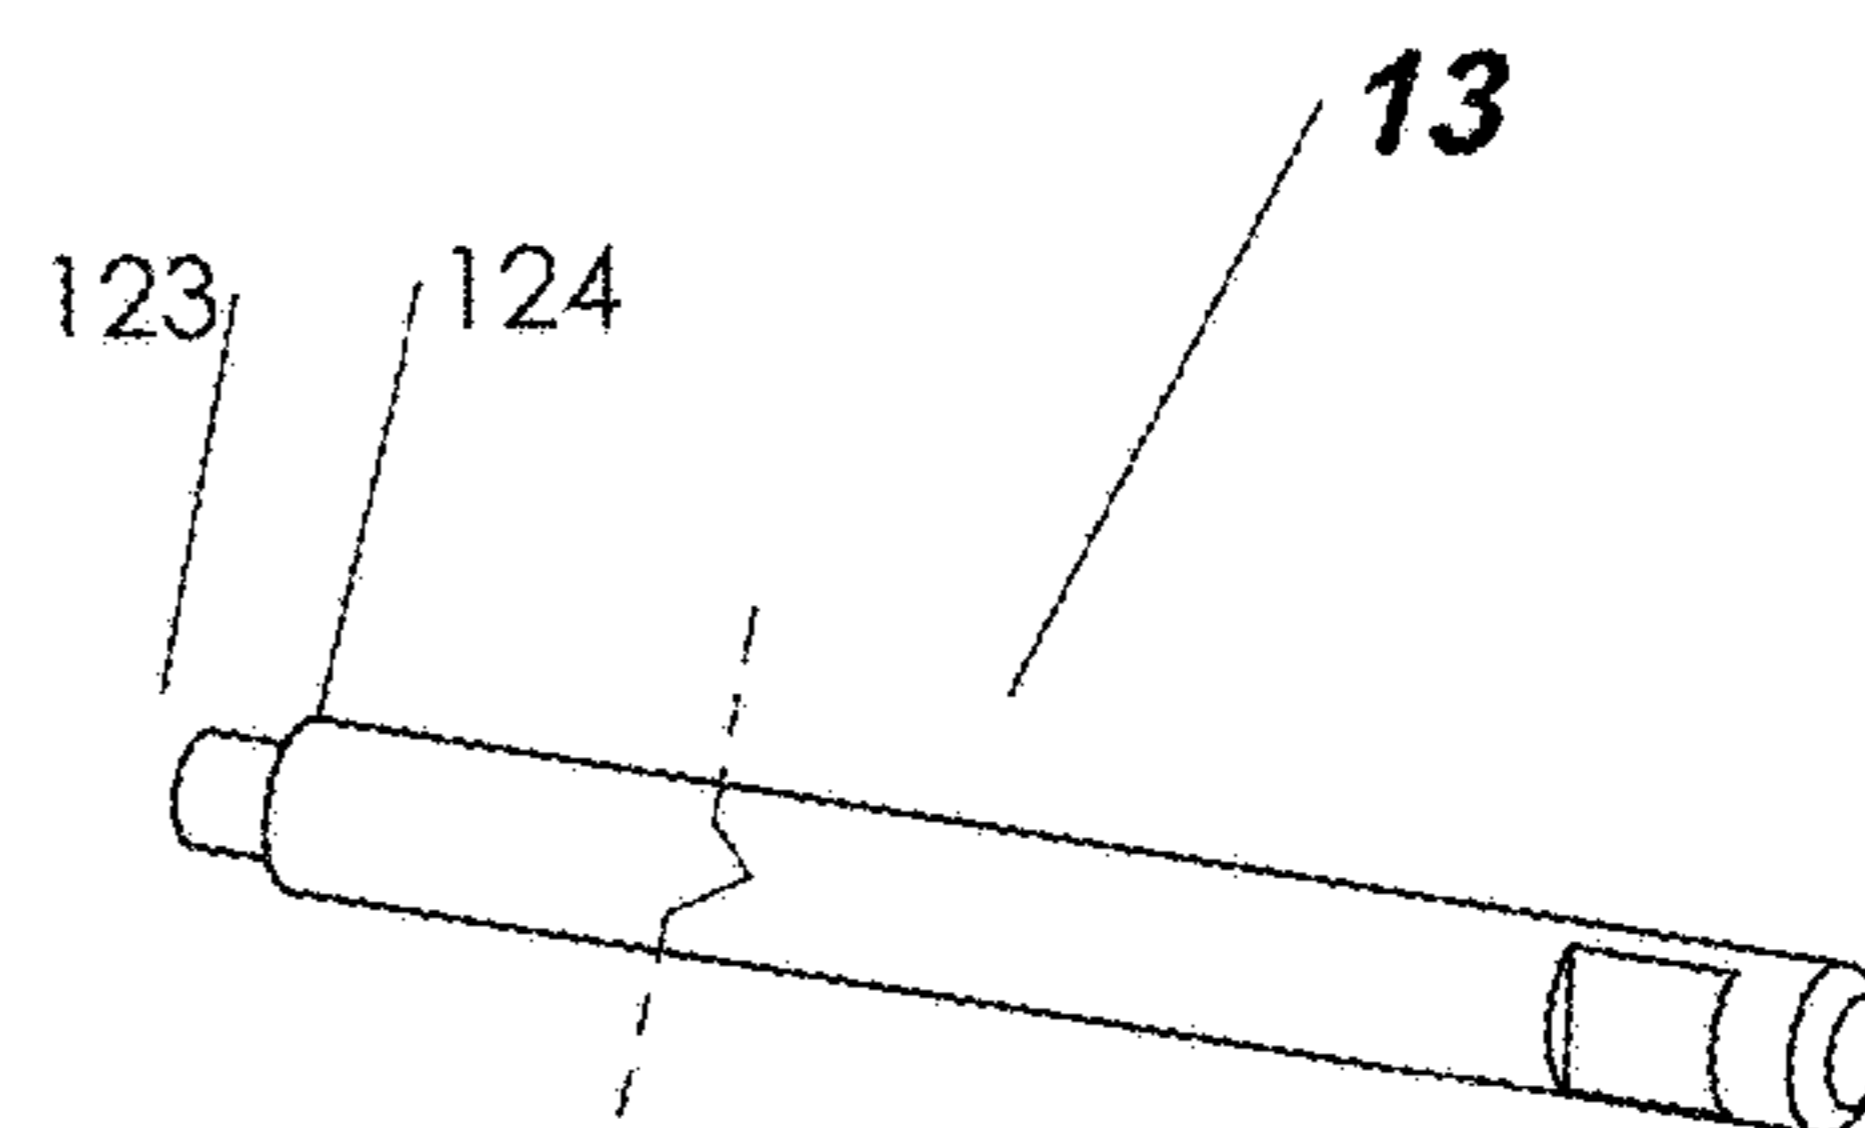


Fig. 21

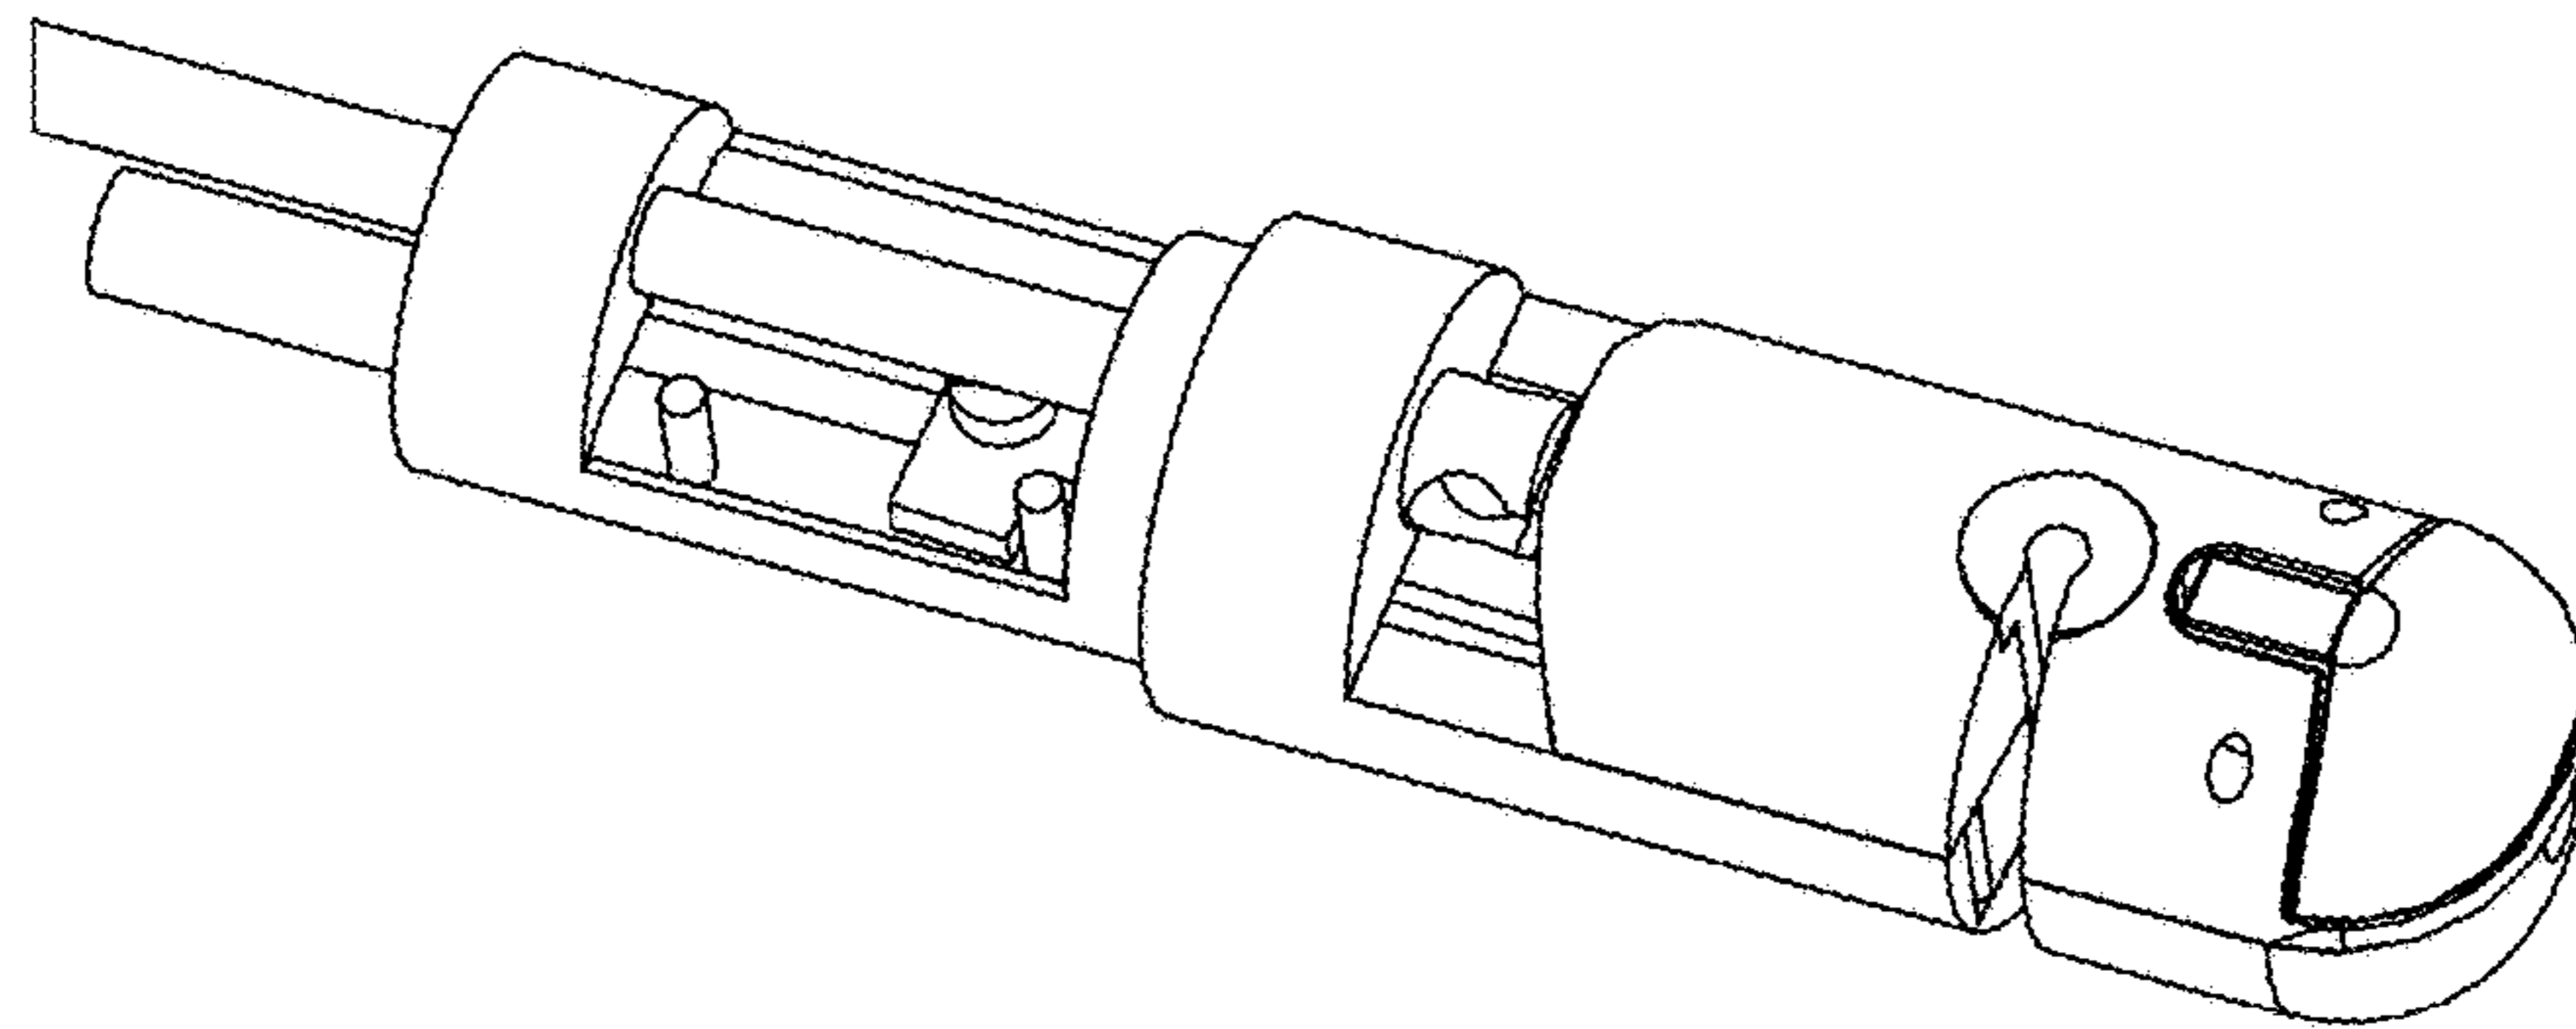


Fig. 22

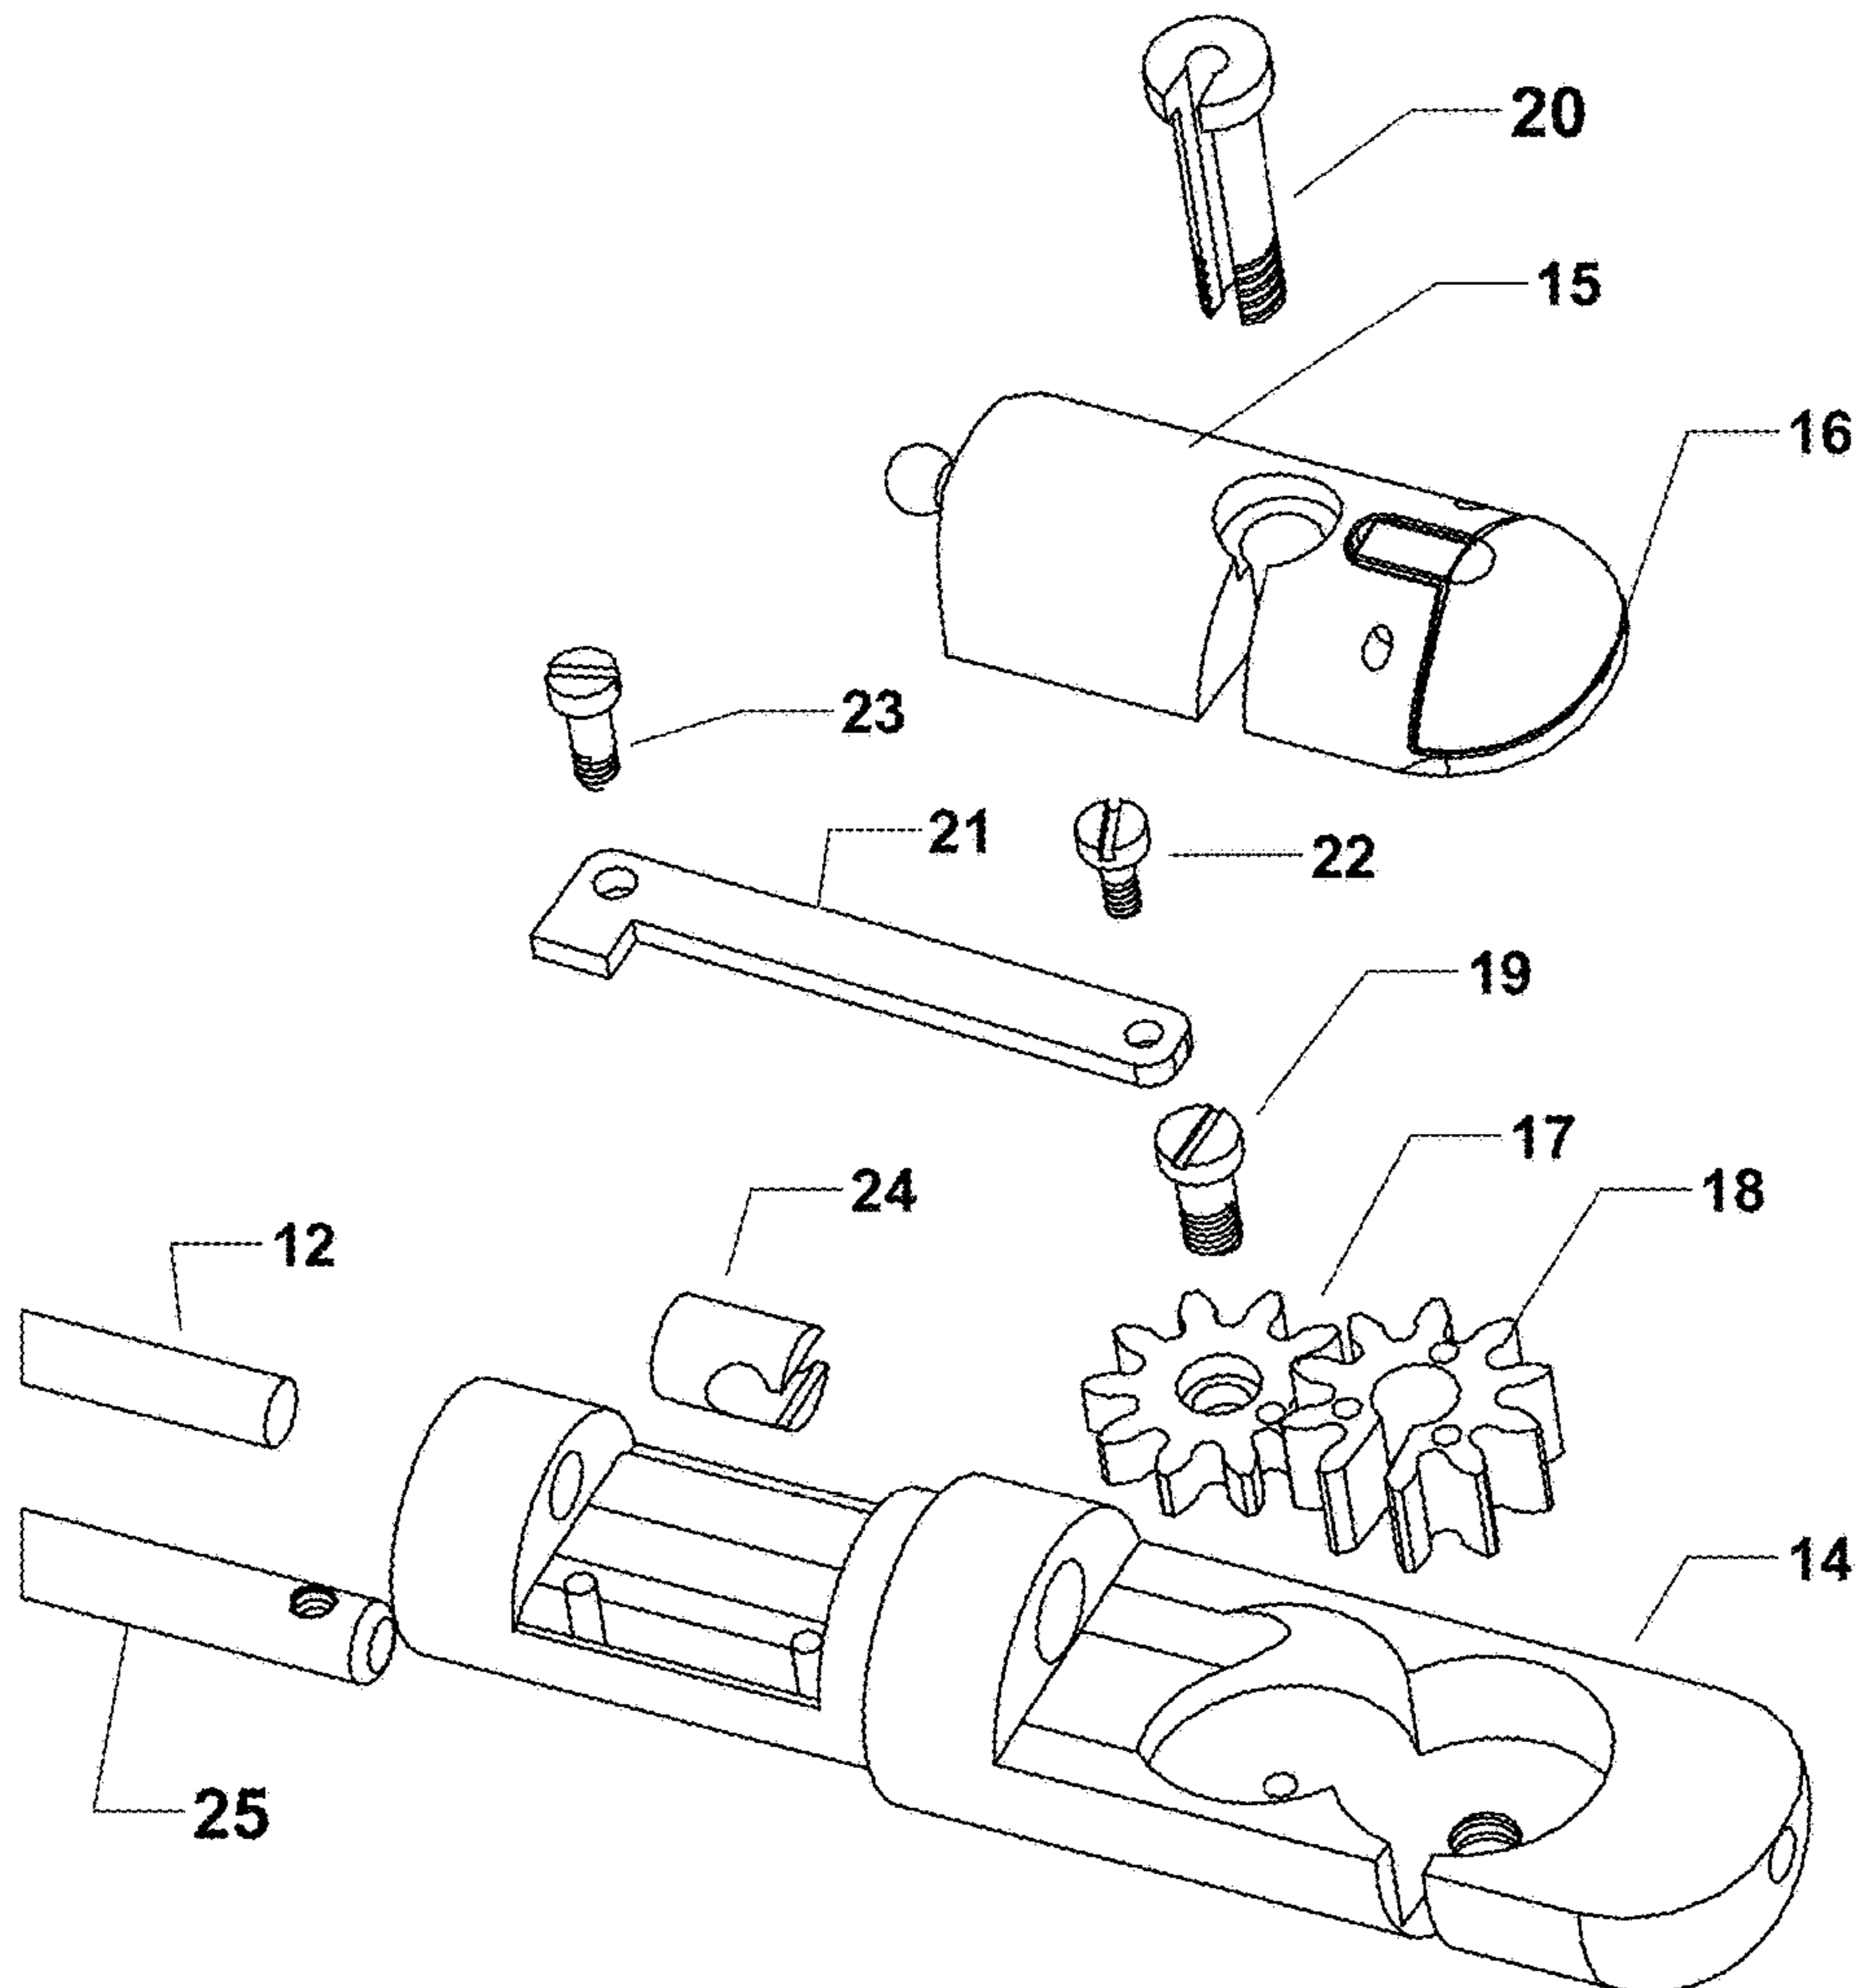


Fig. 23

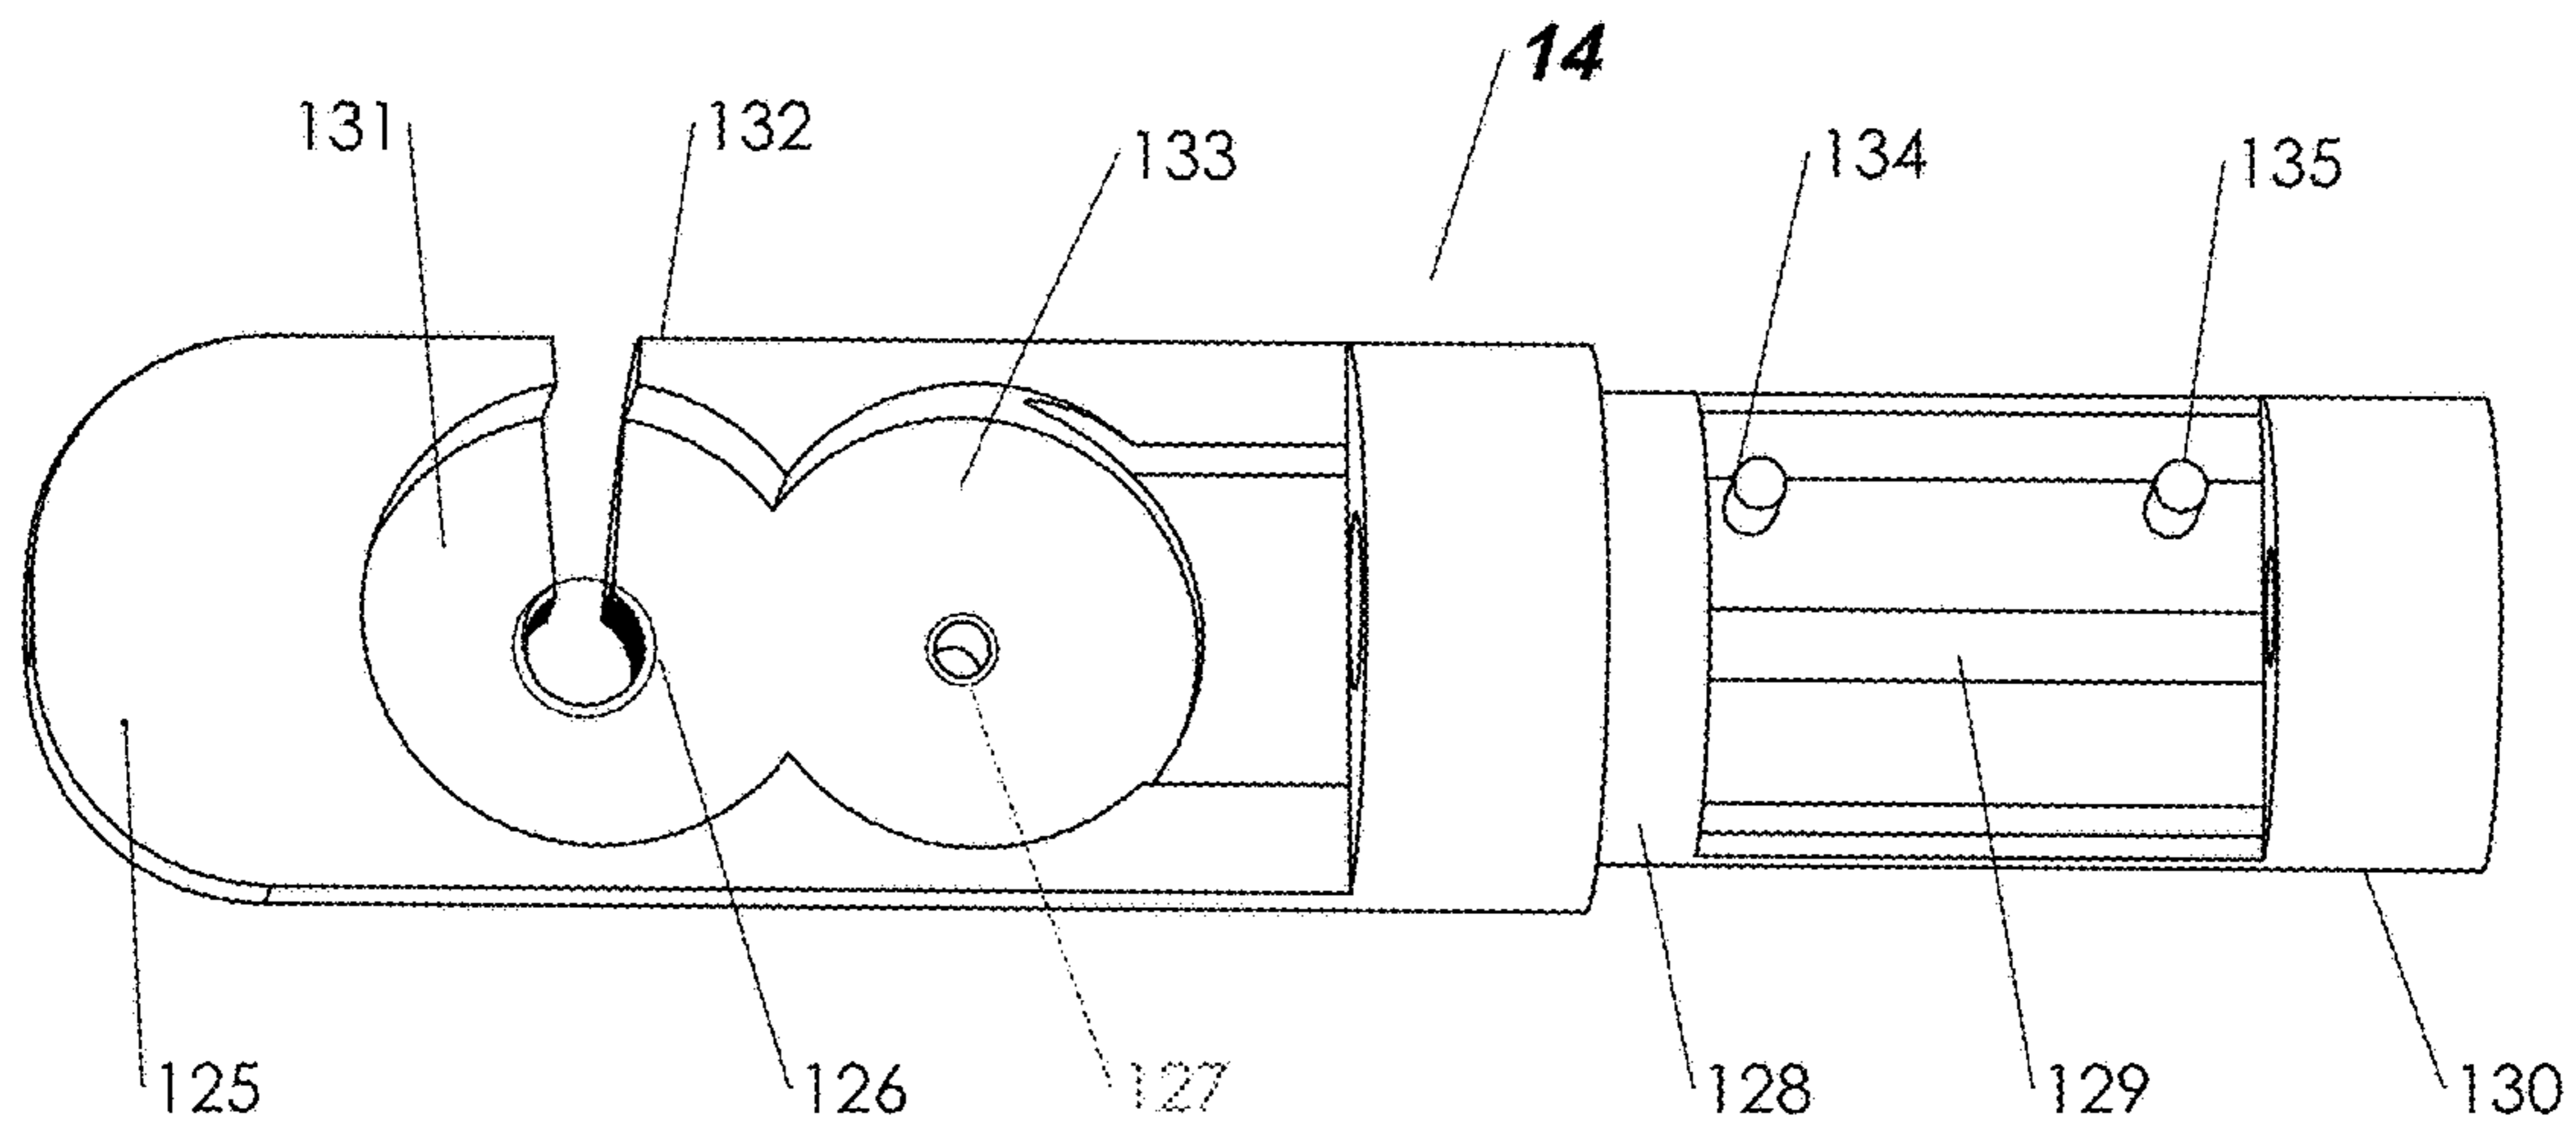


Fig. 24

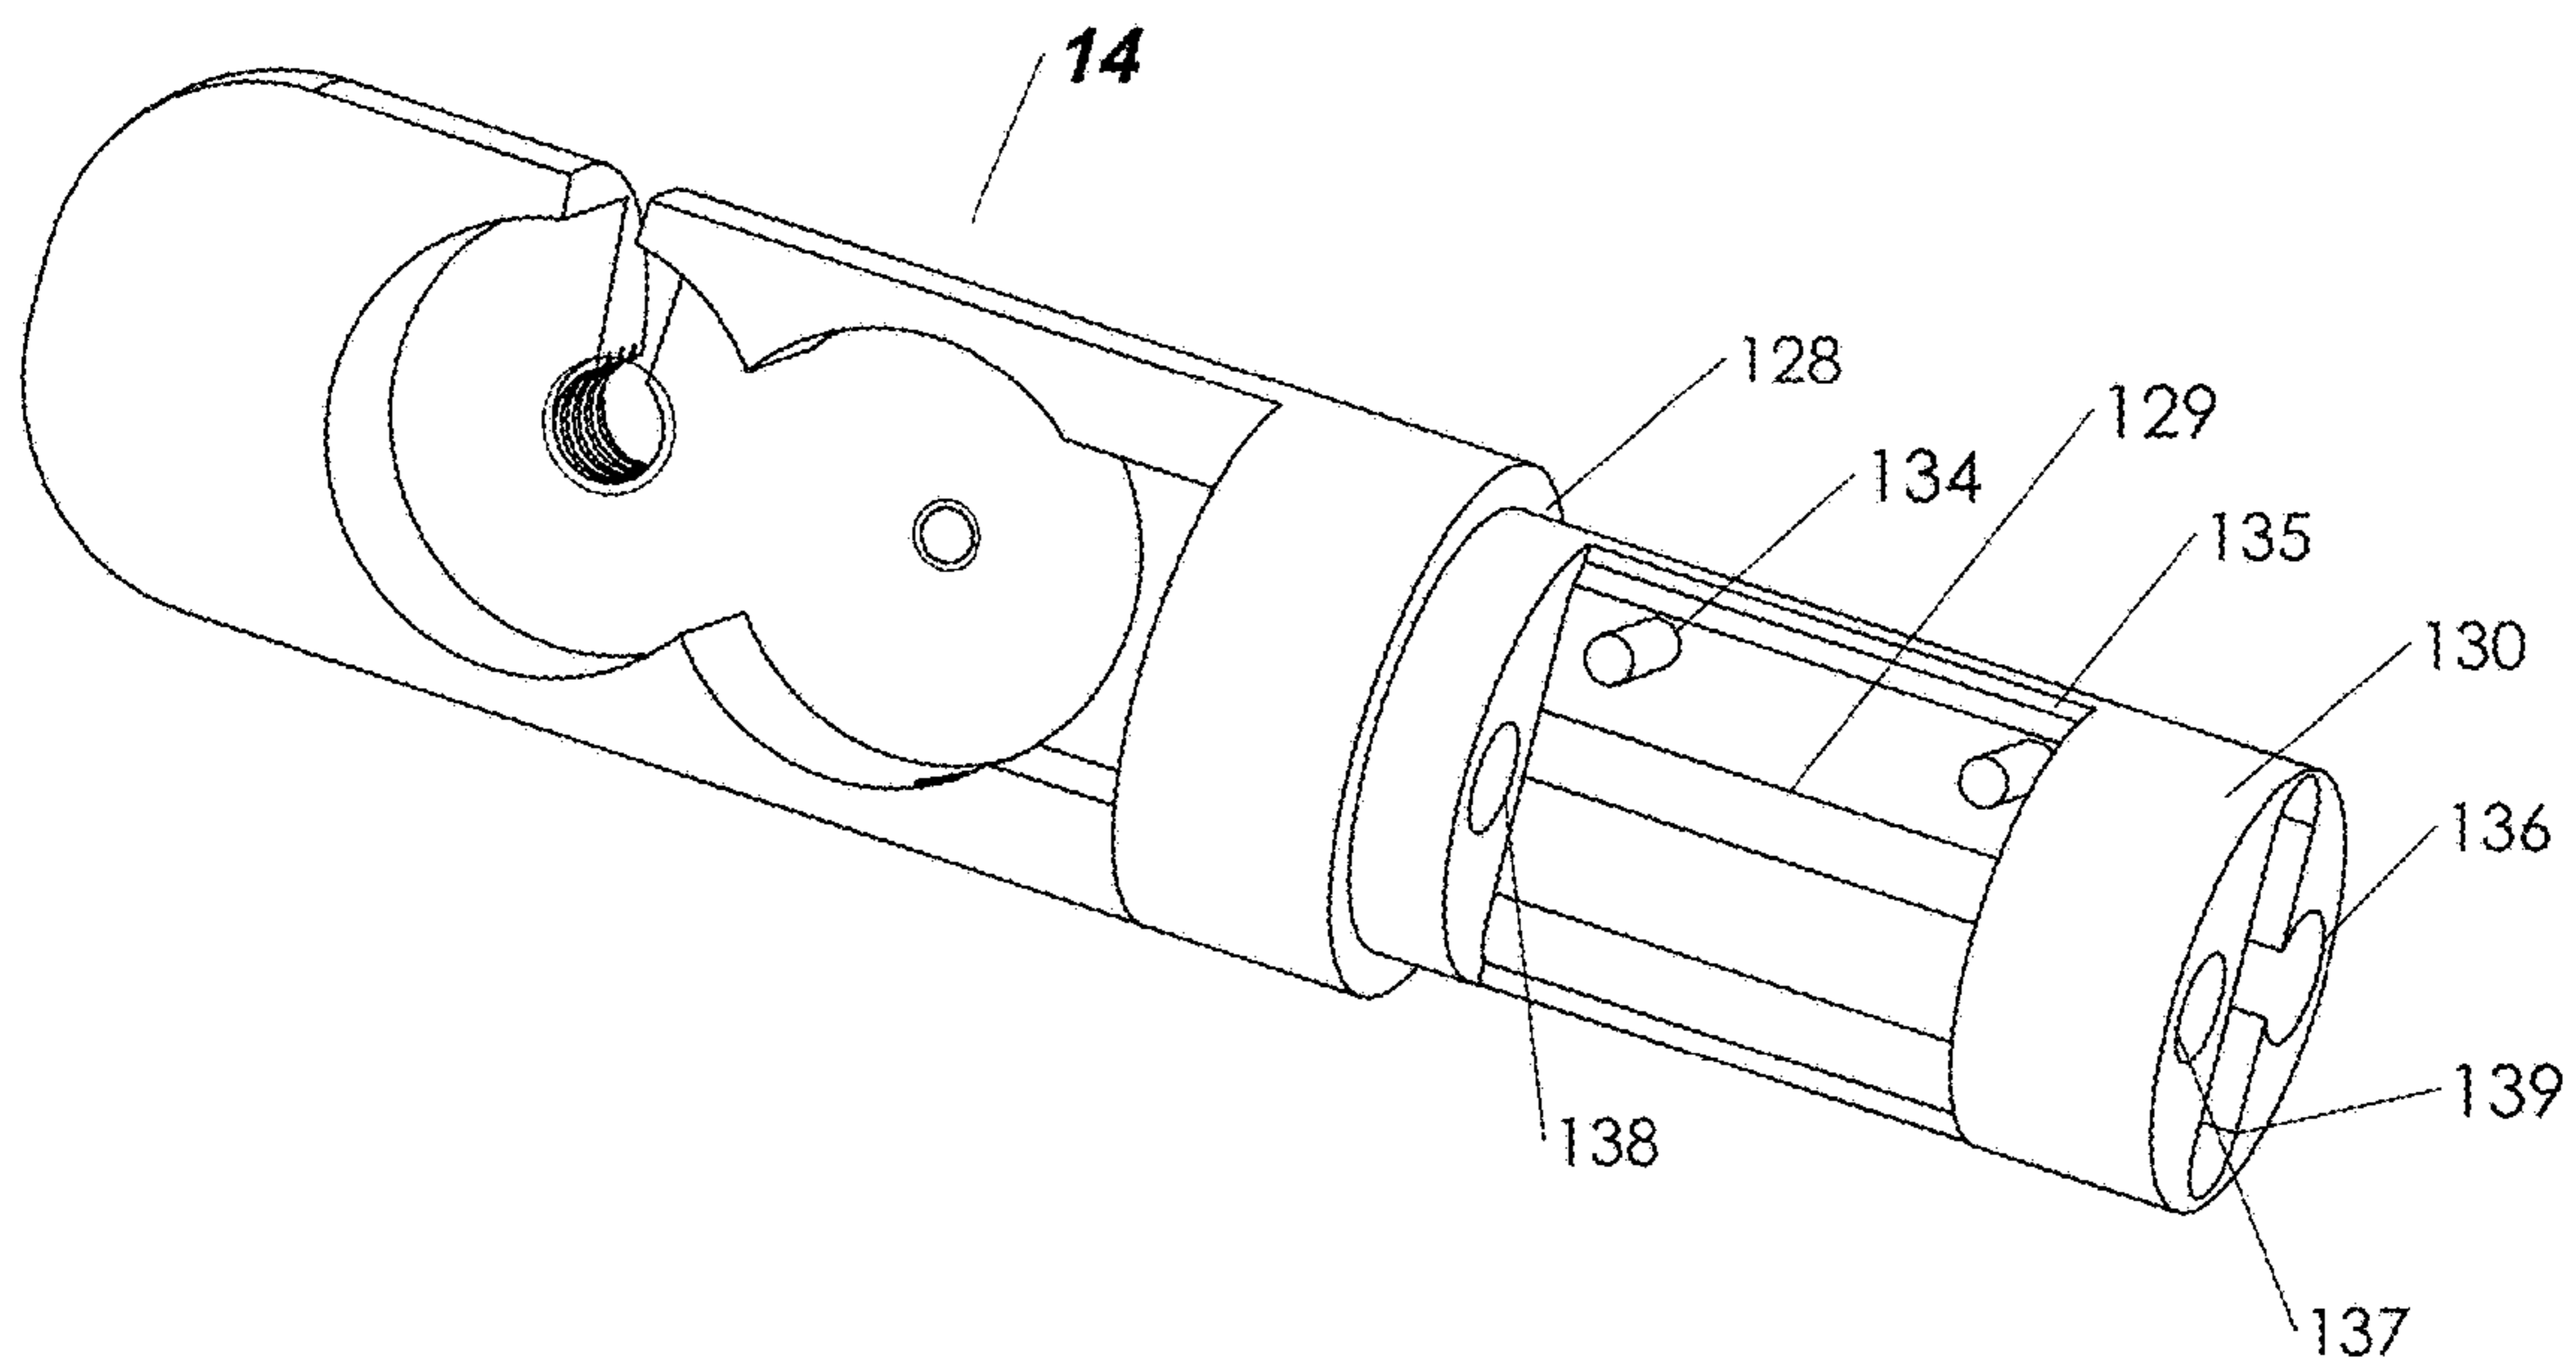


Fig. 25

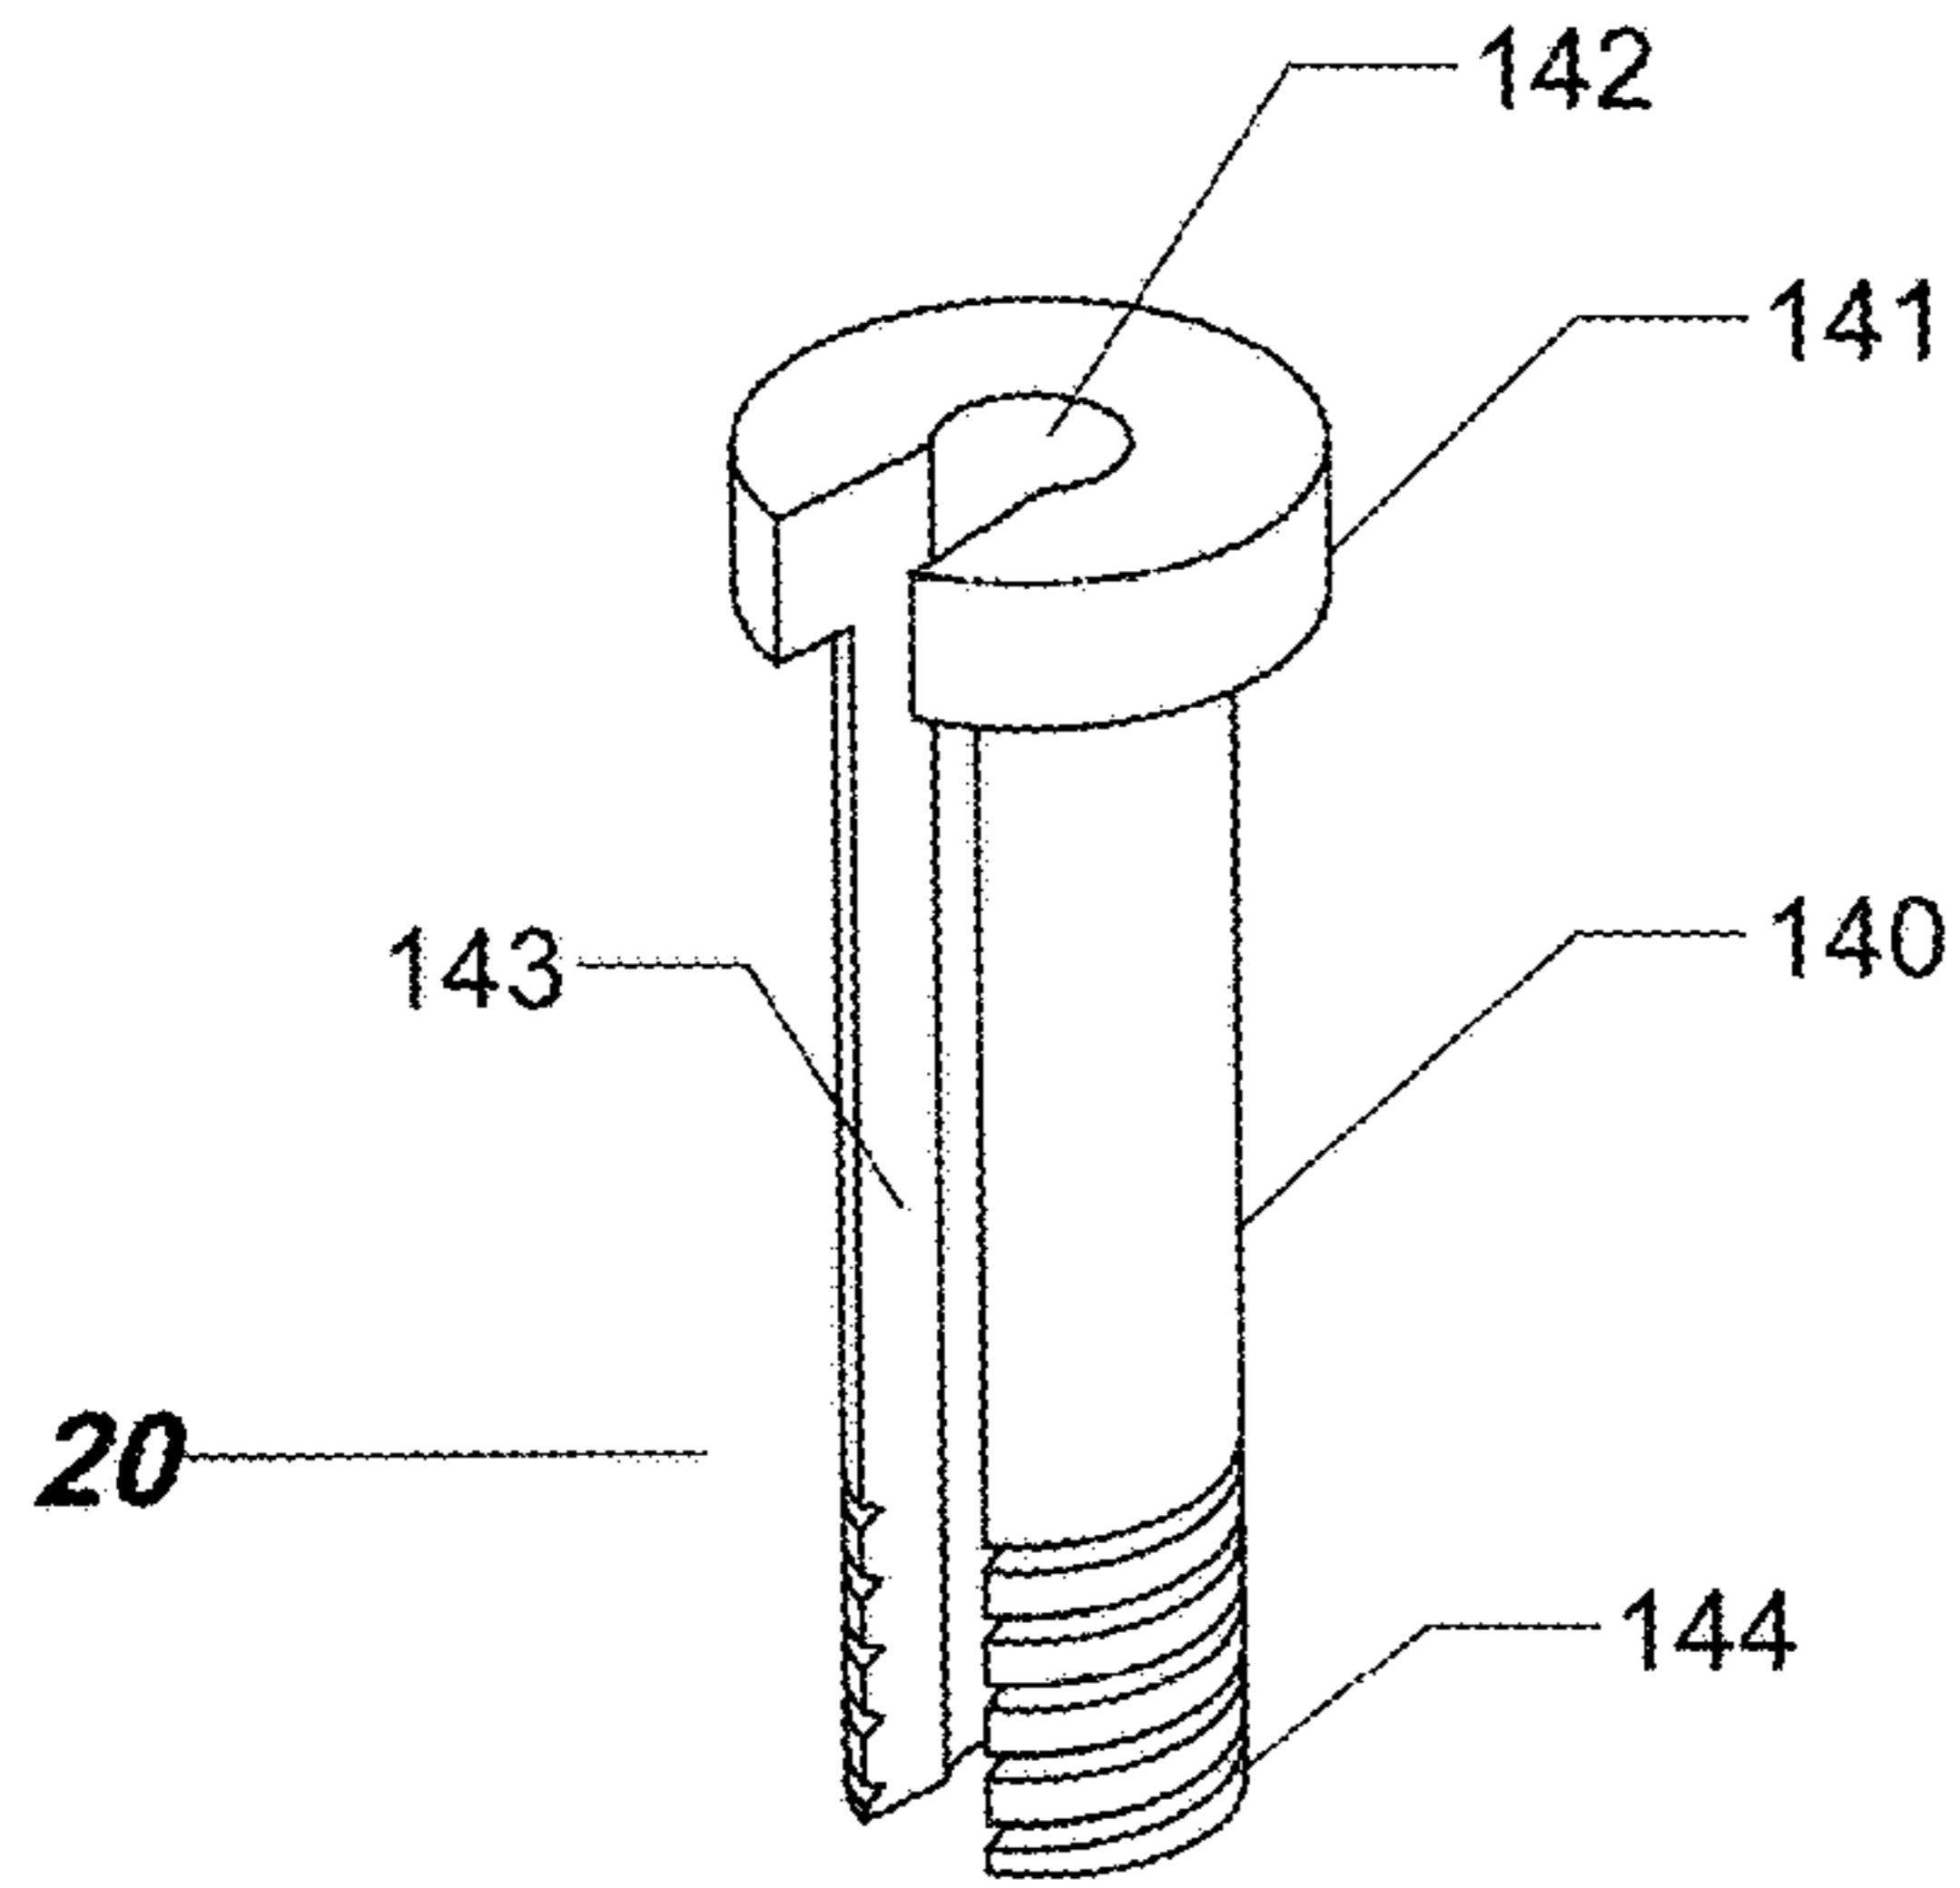


Fig. 26

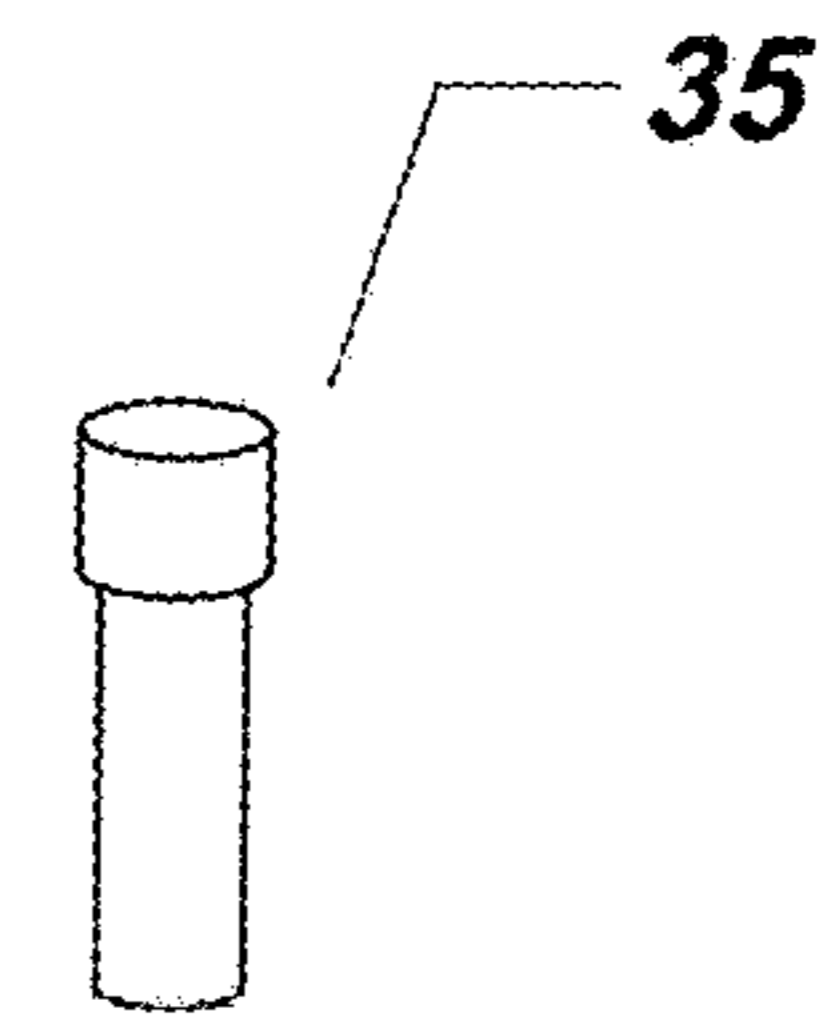


Fig. 27

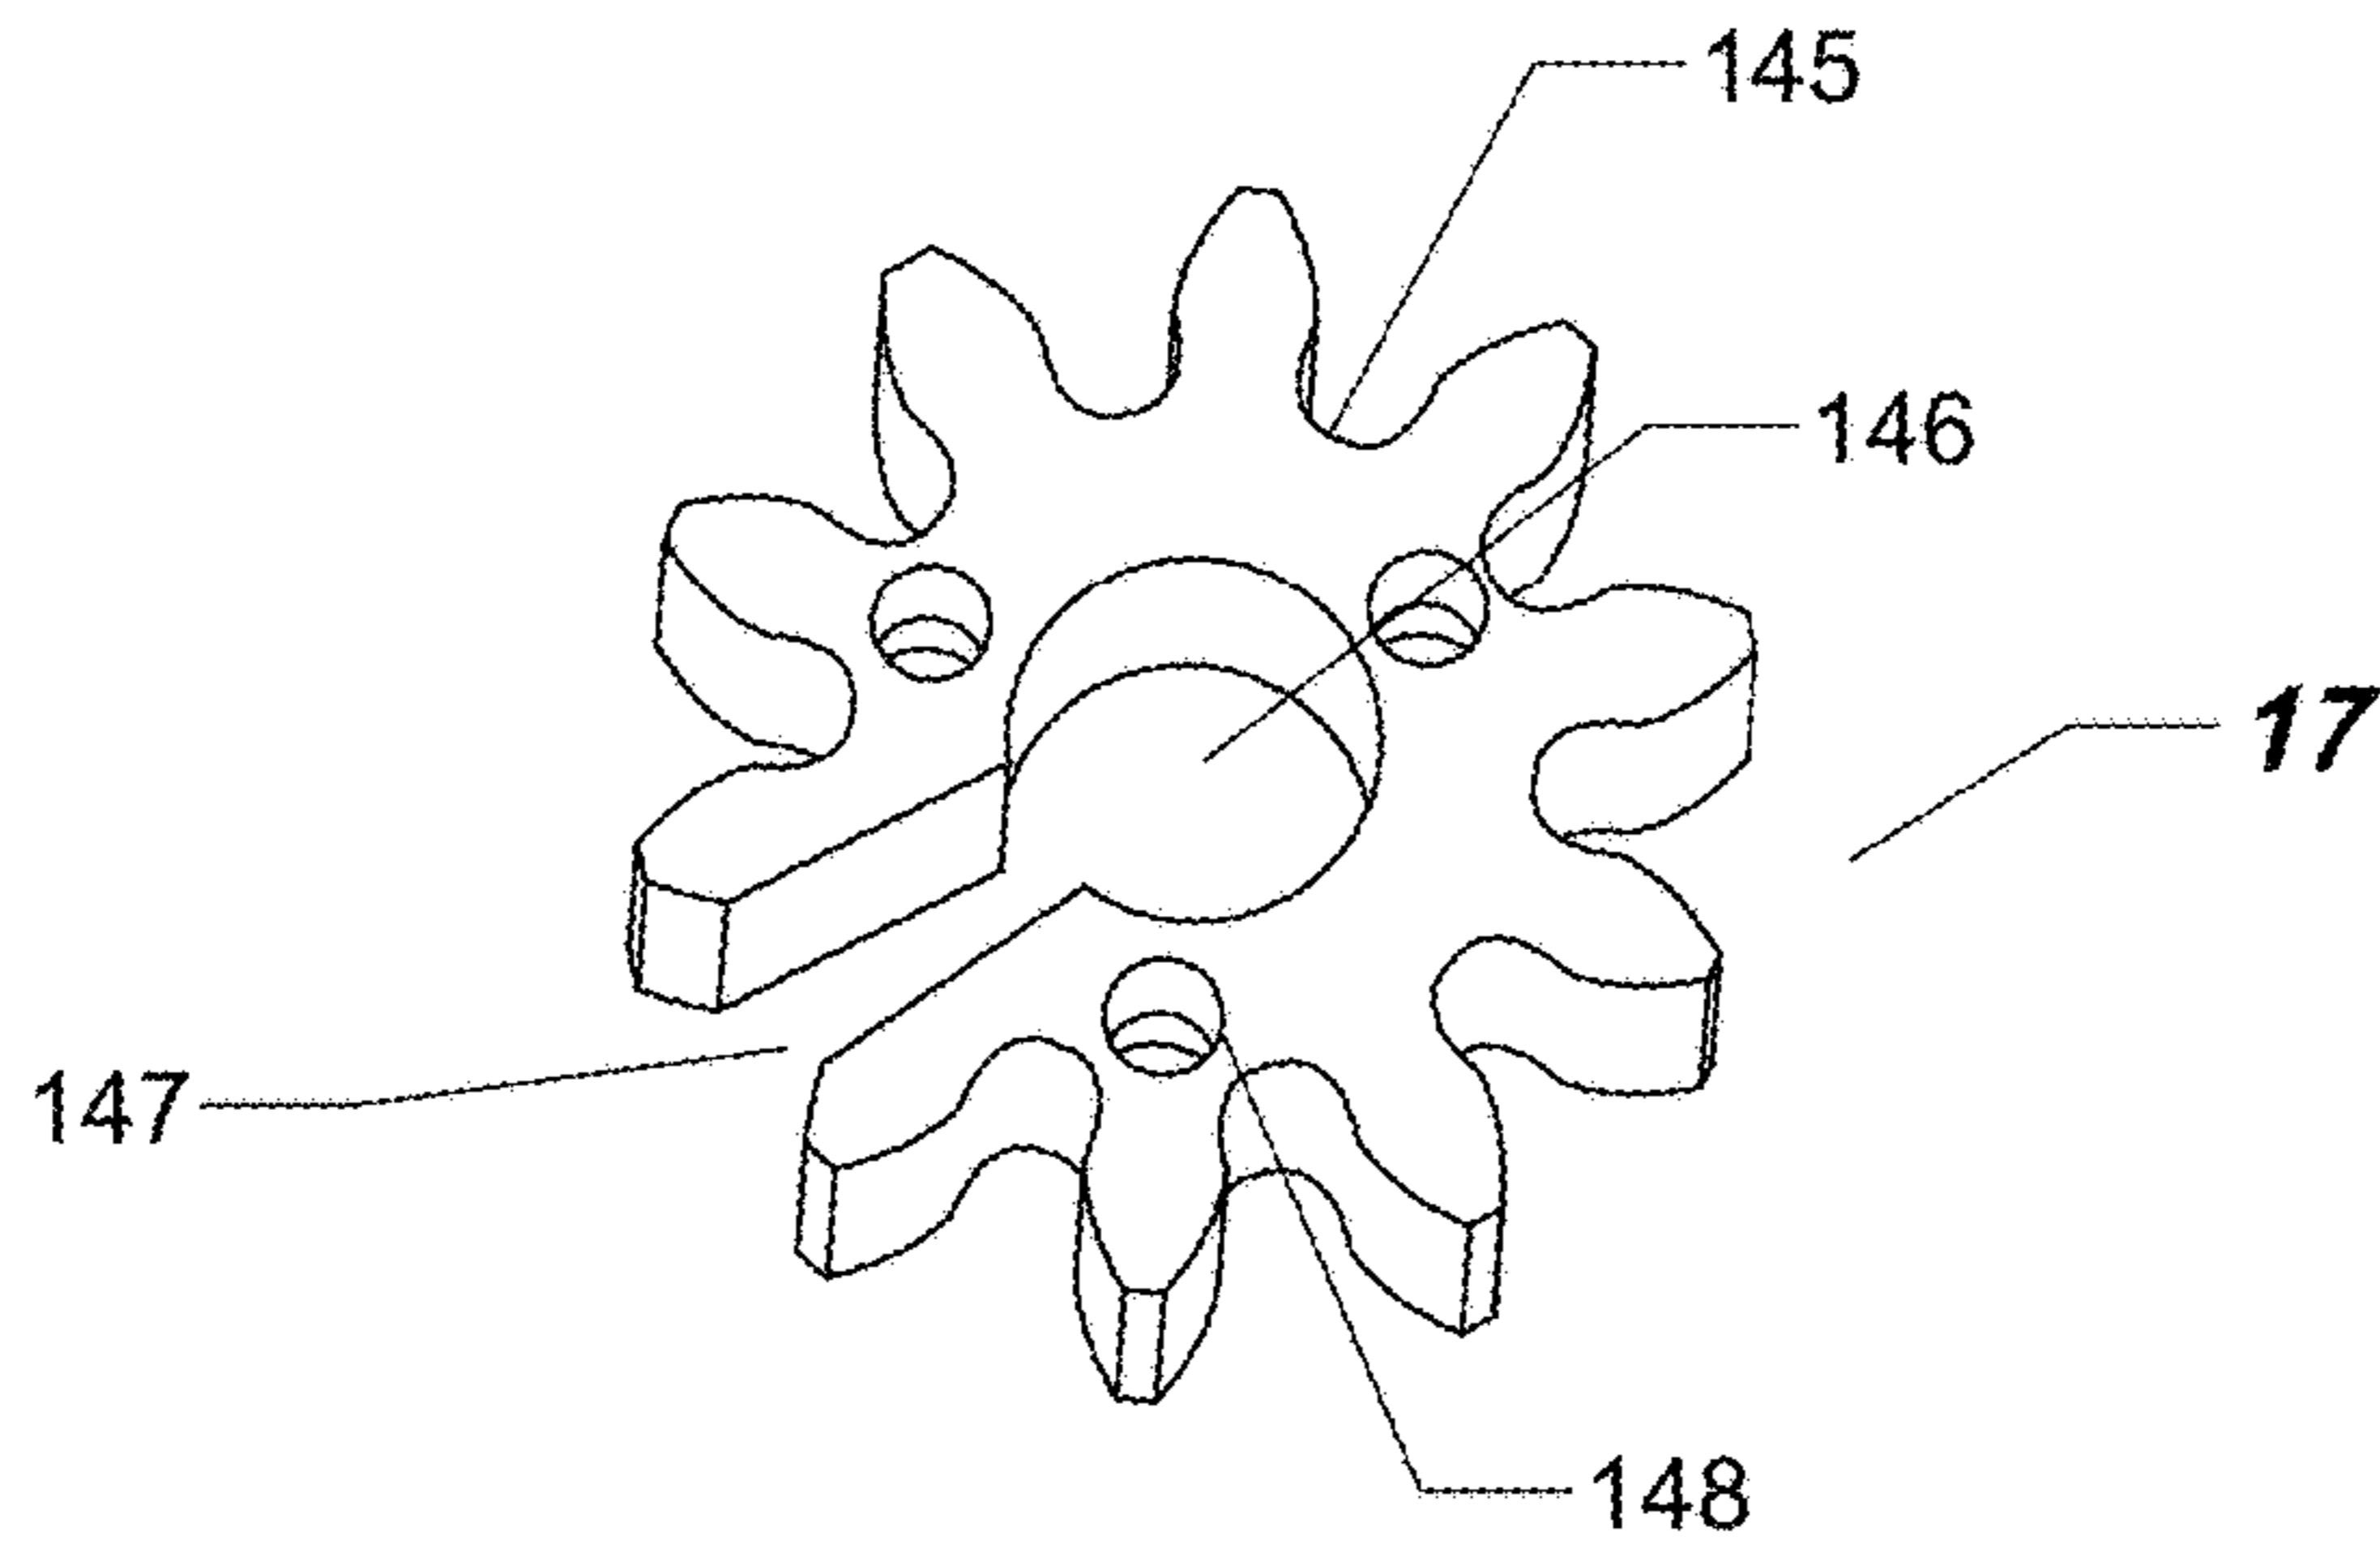


Fig. 28

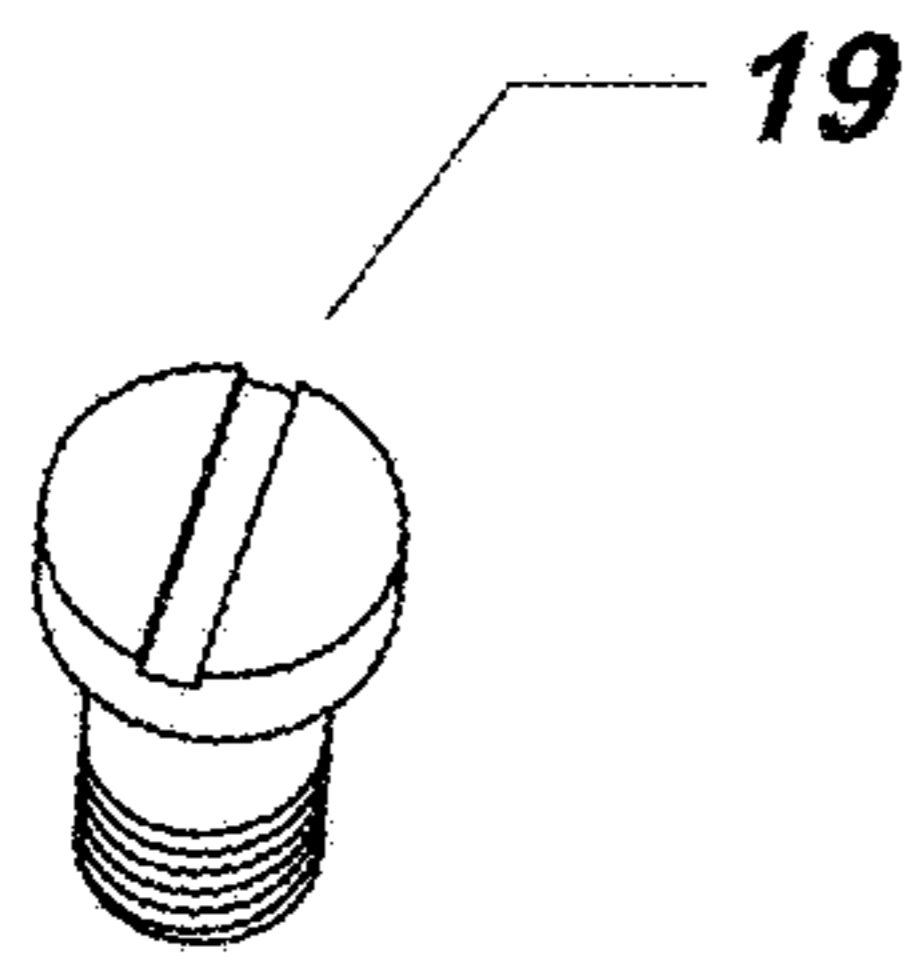


Fig. 29

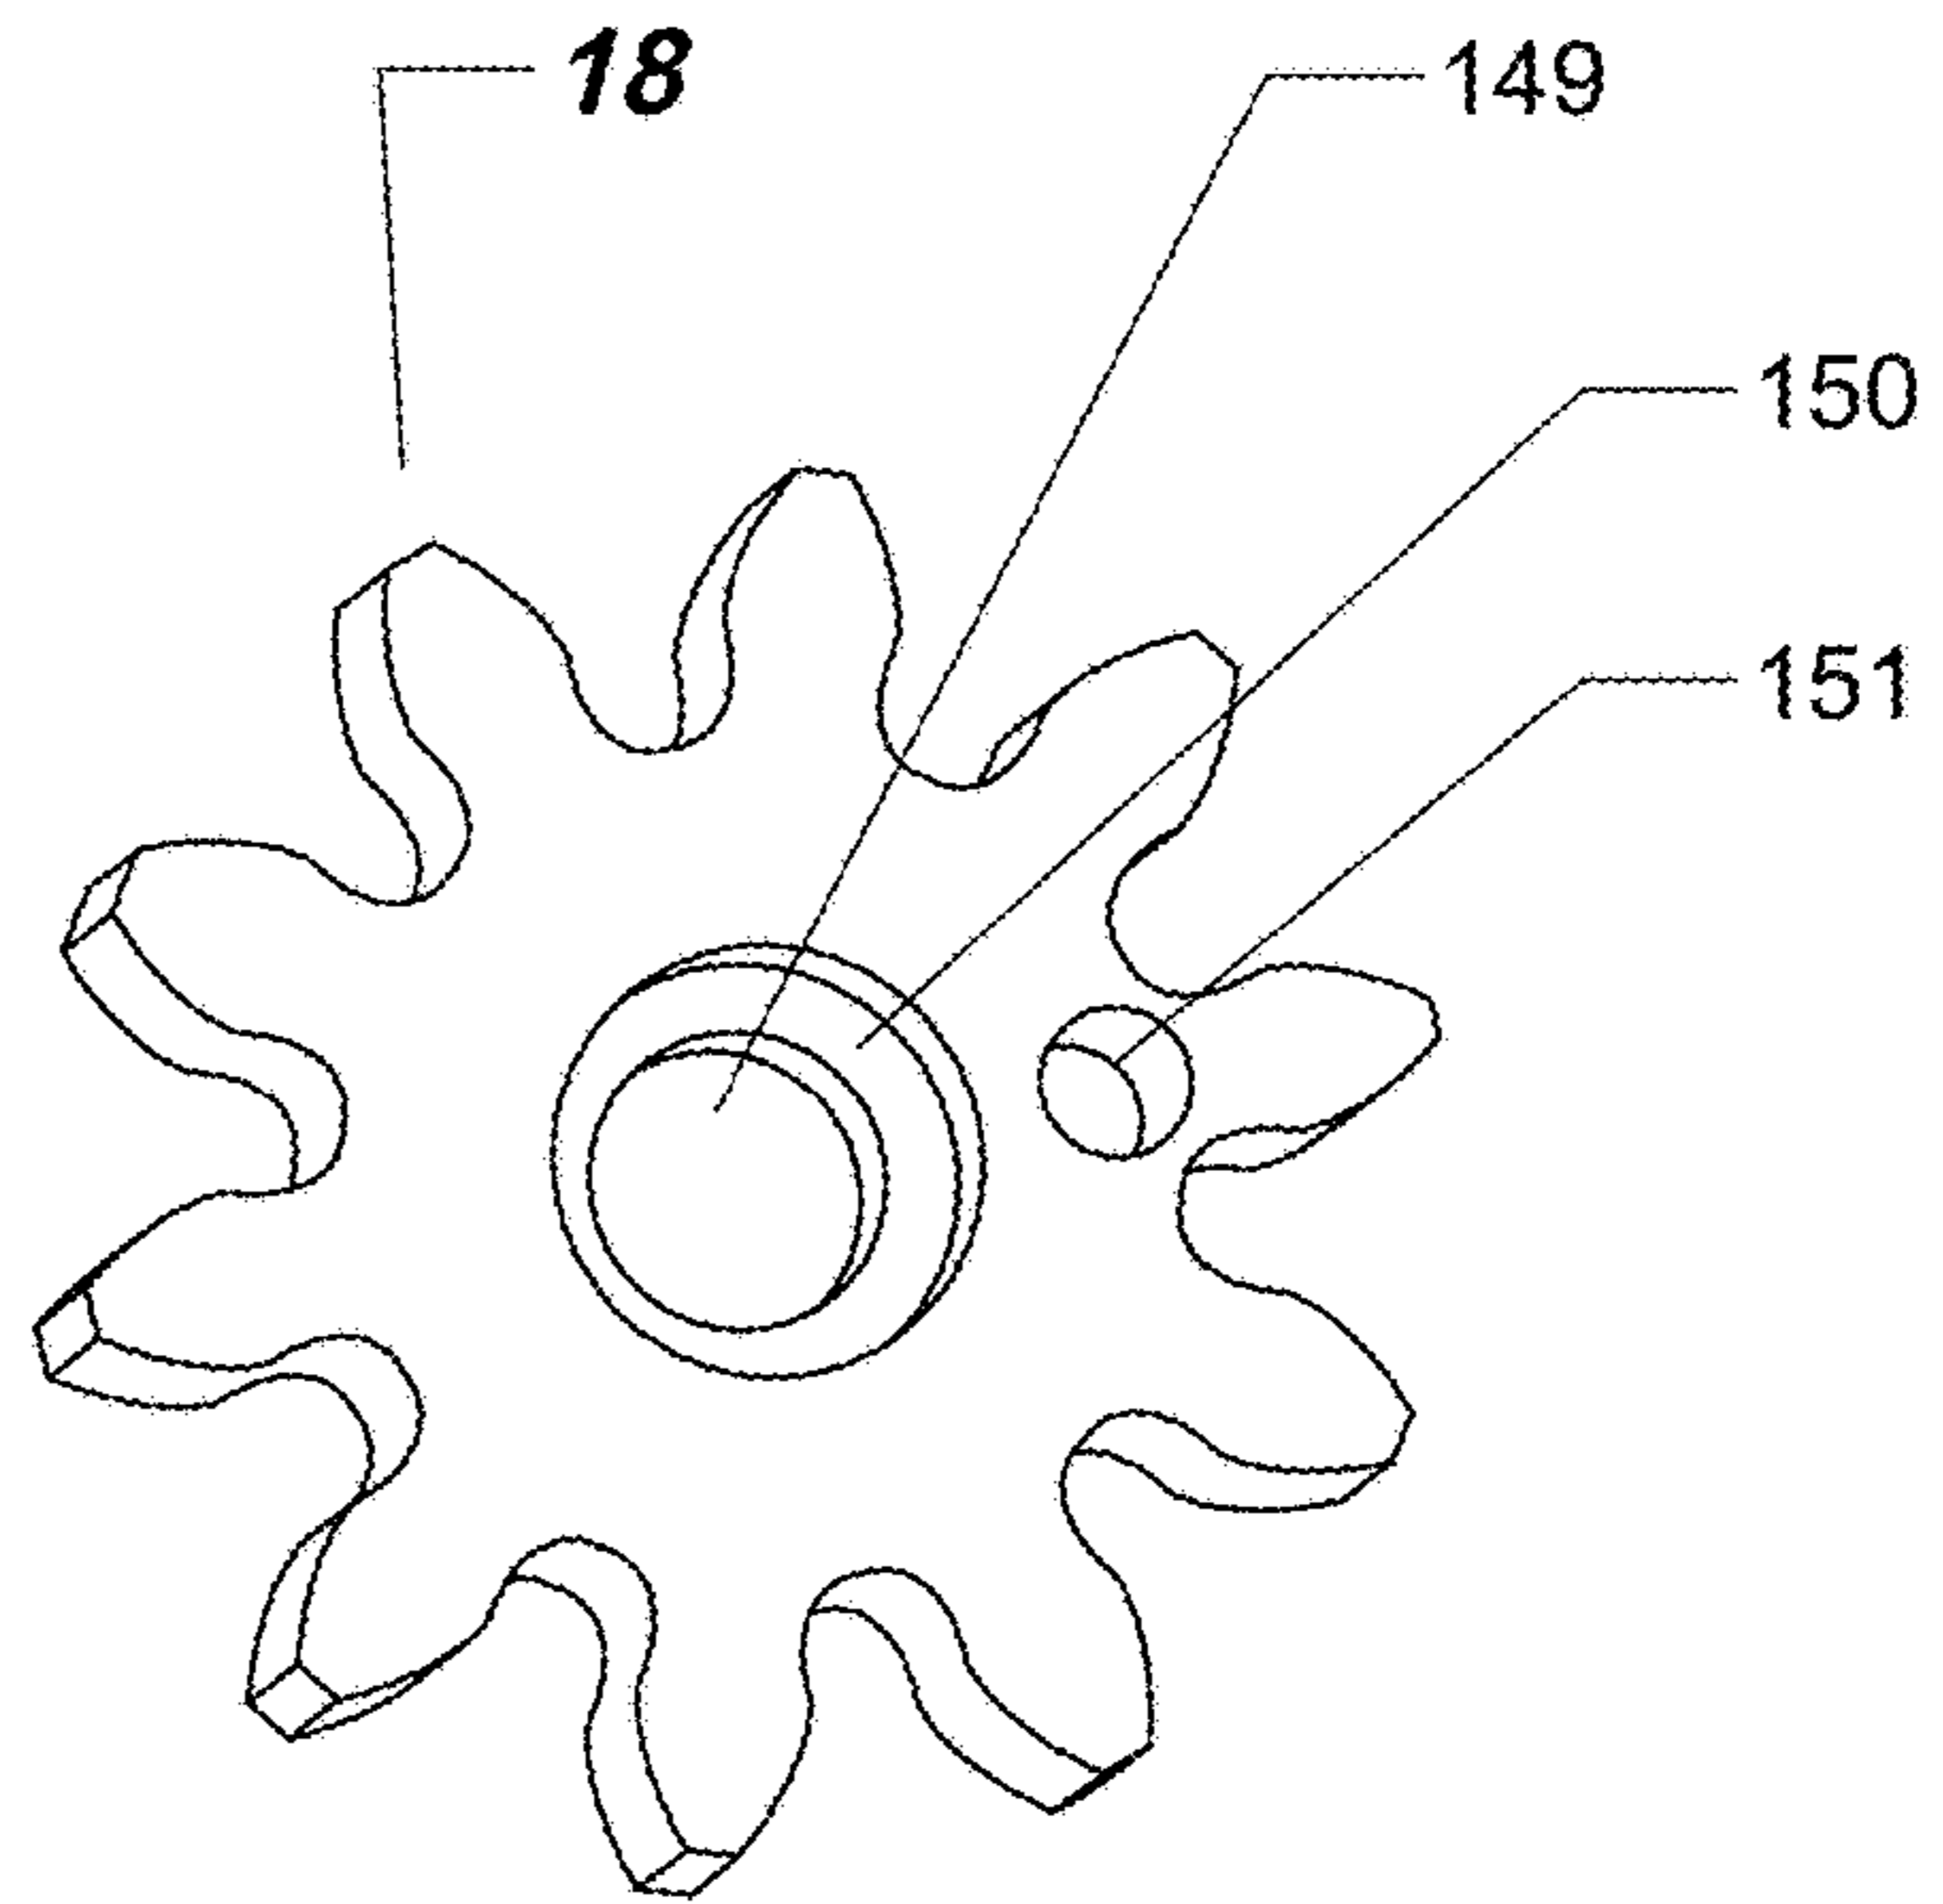


Fig. 30

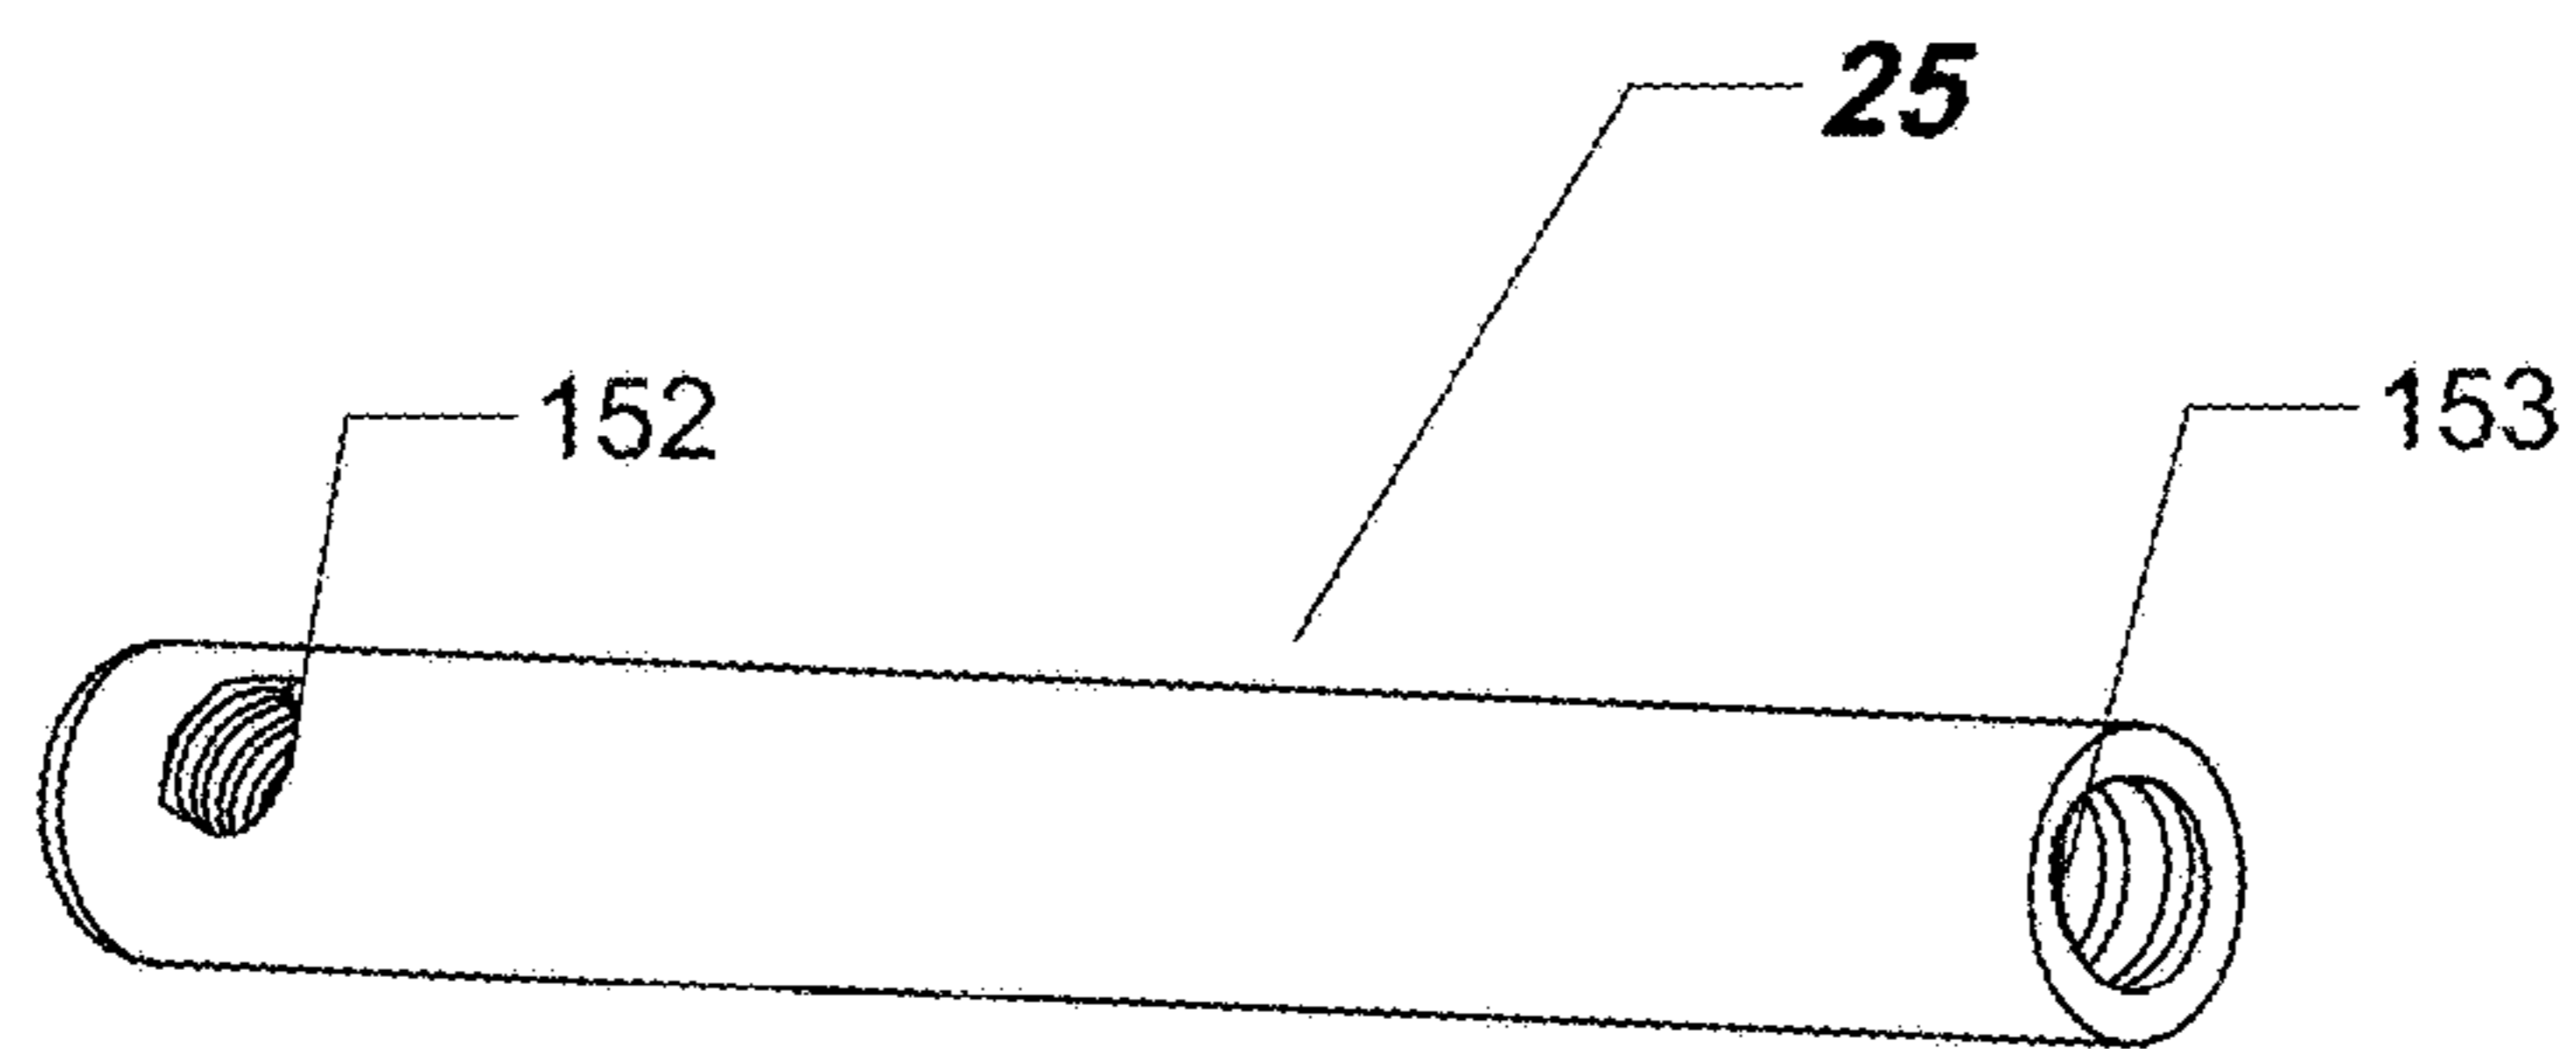


Fig. 31

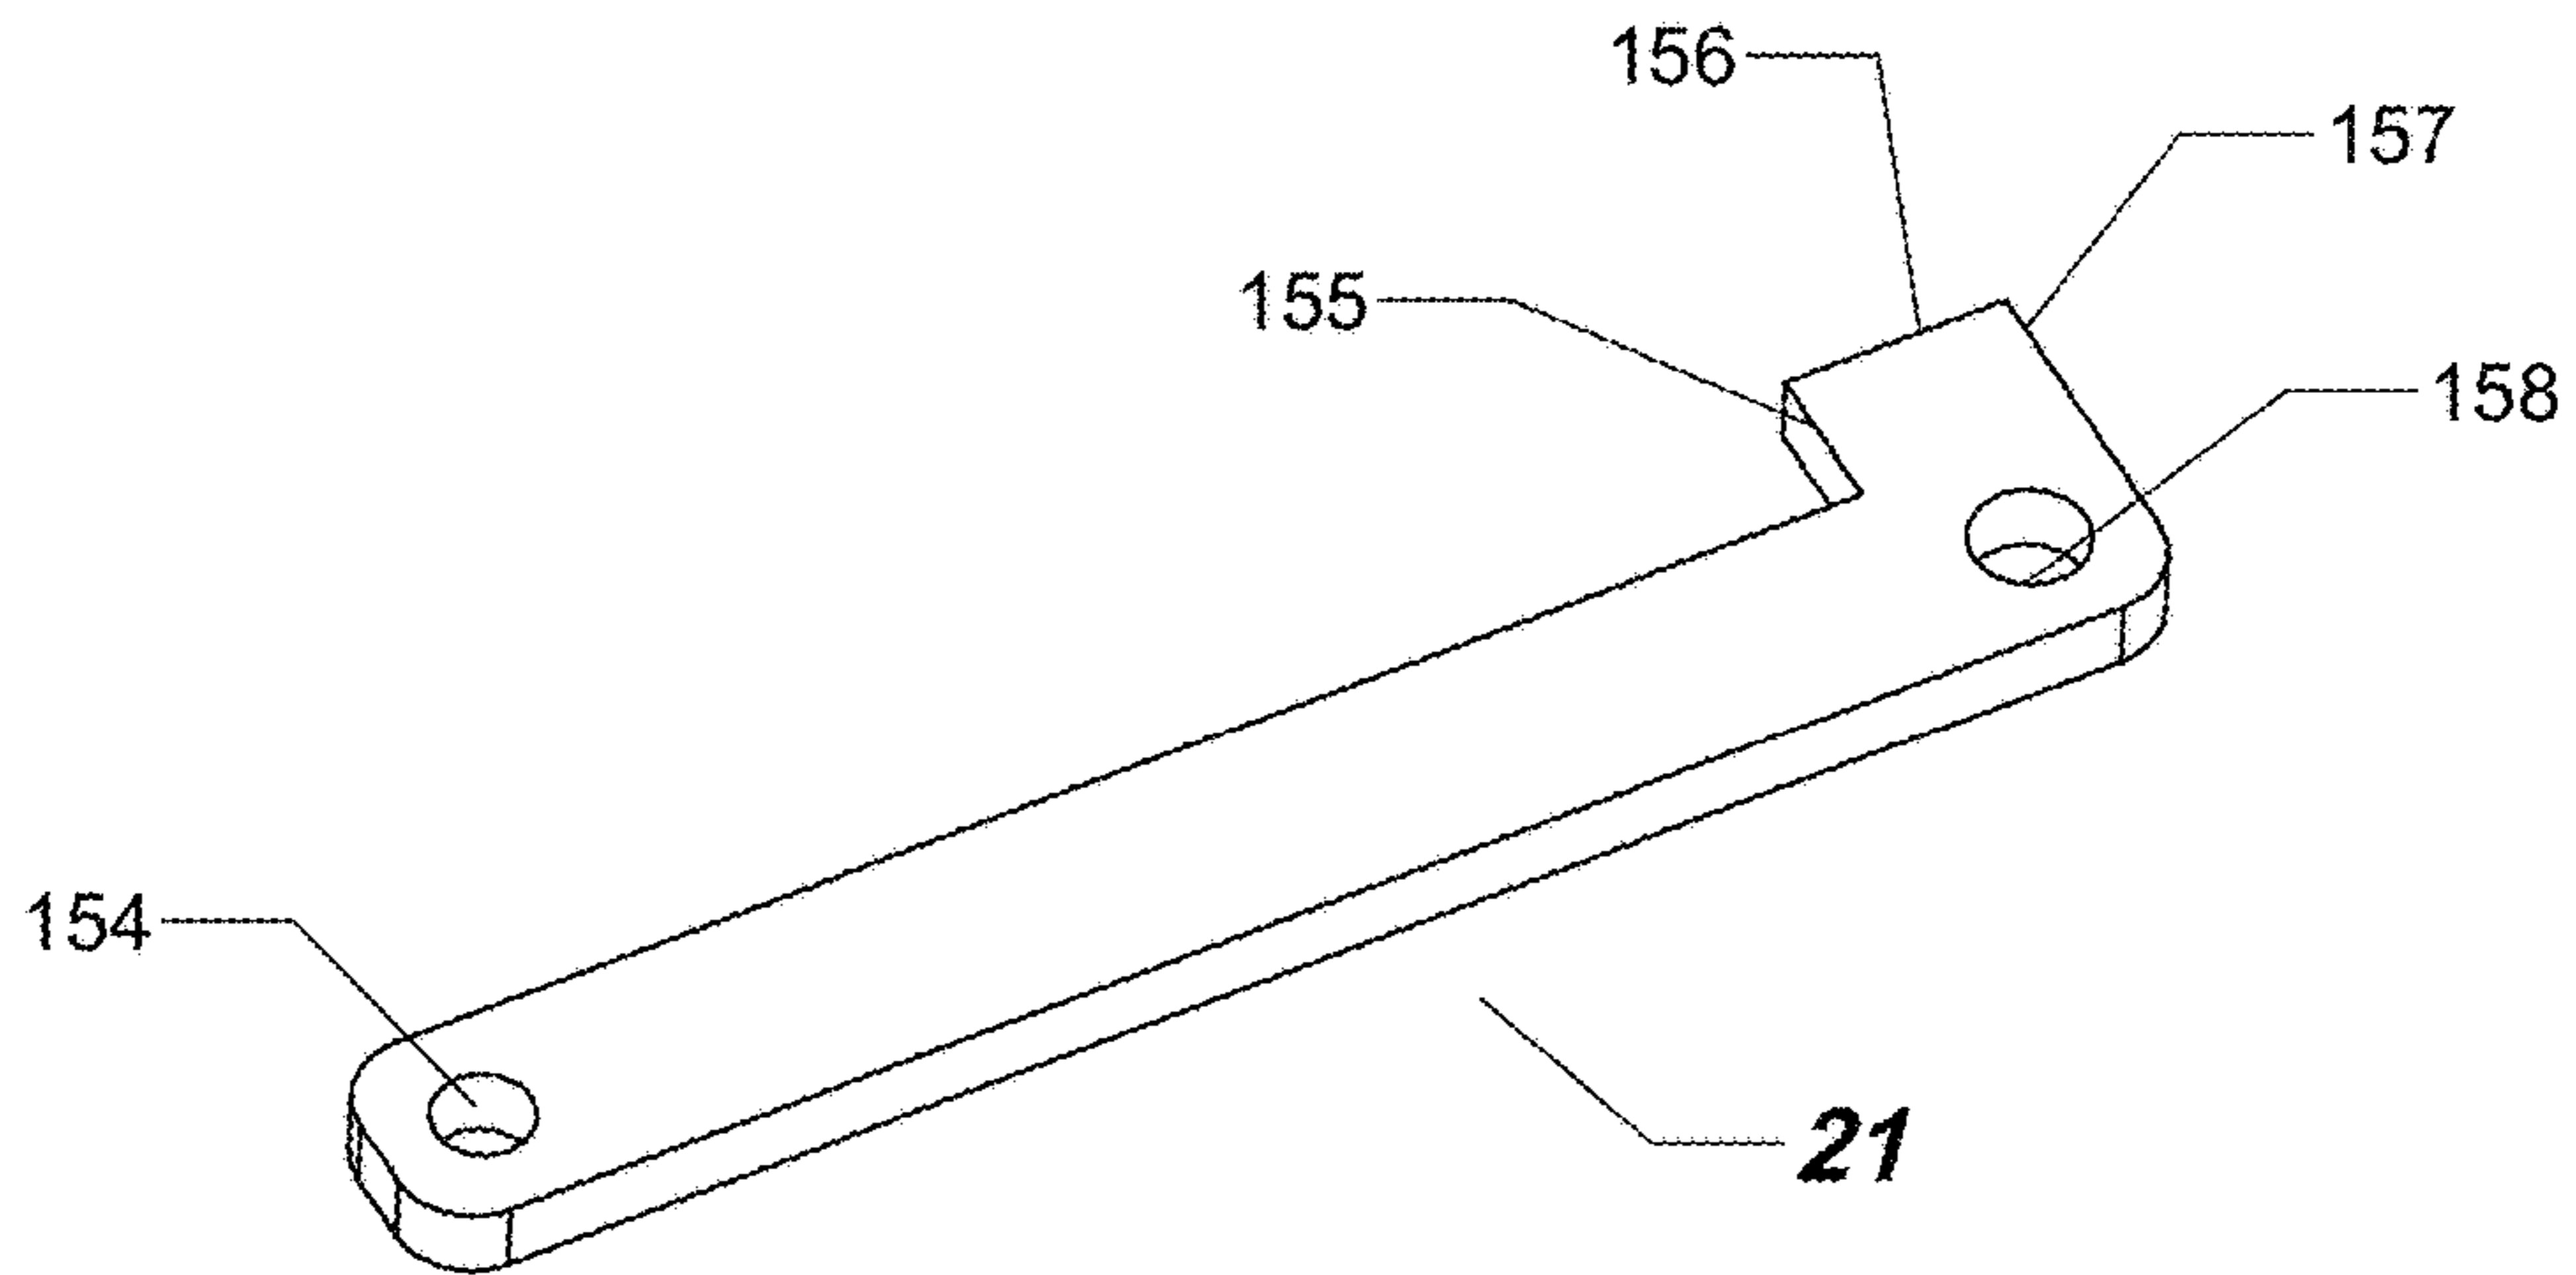


Fig. 32

PRIOR ART

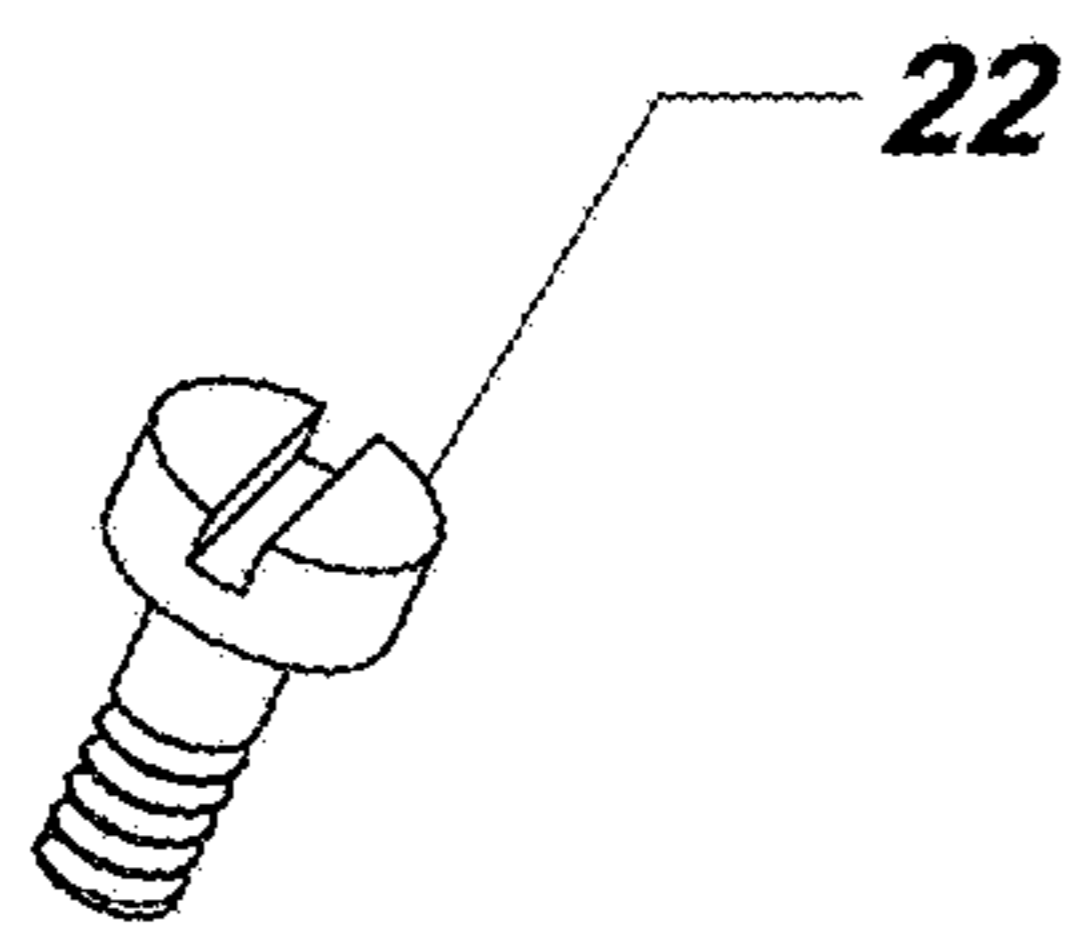


Fig. 33

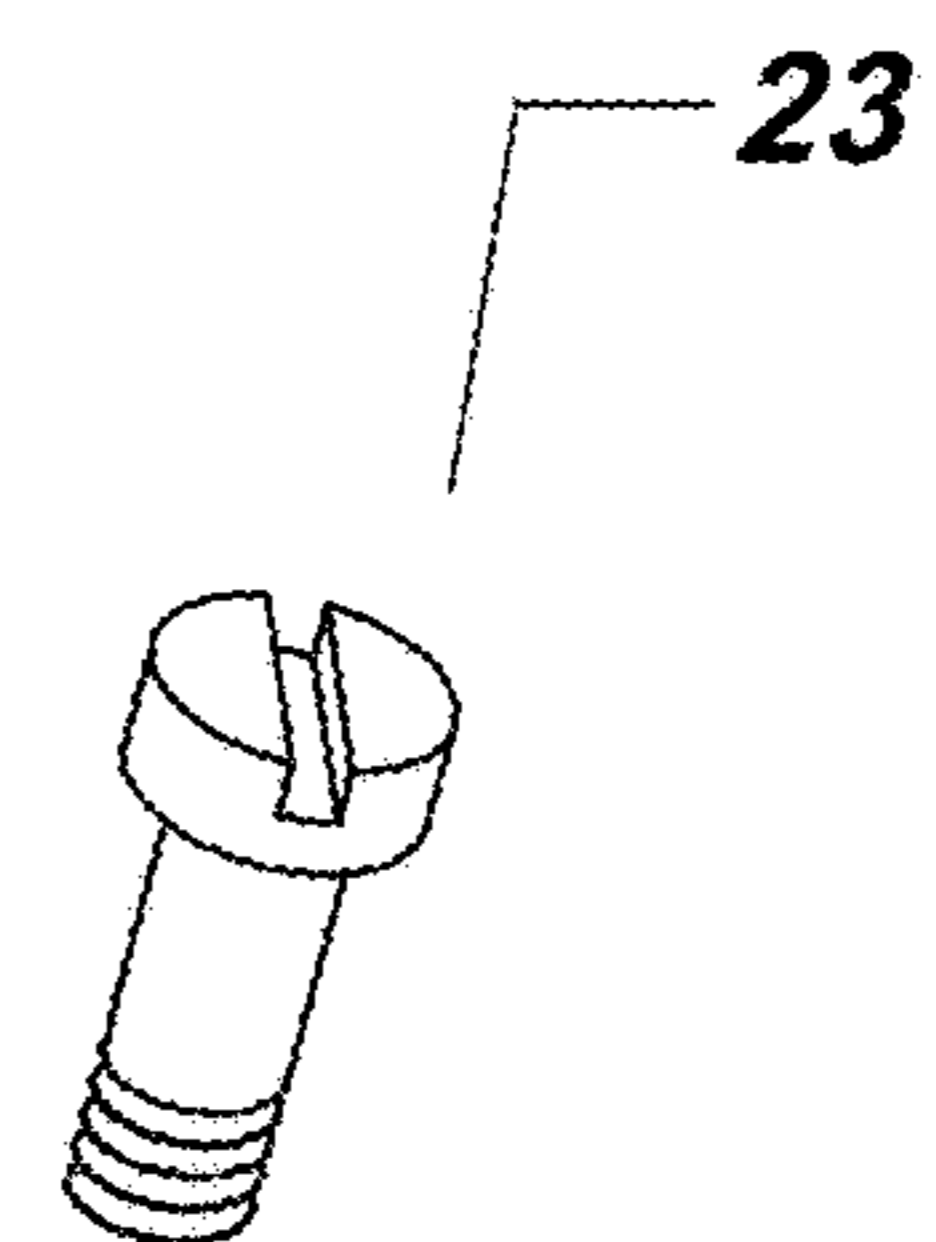


Fig. 34

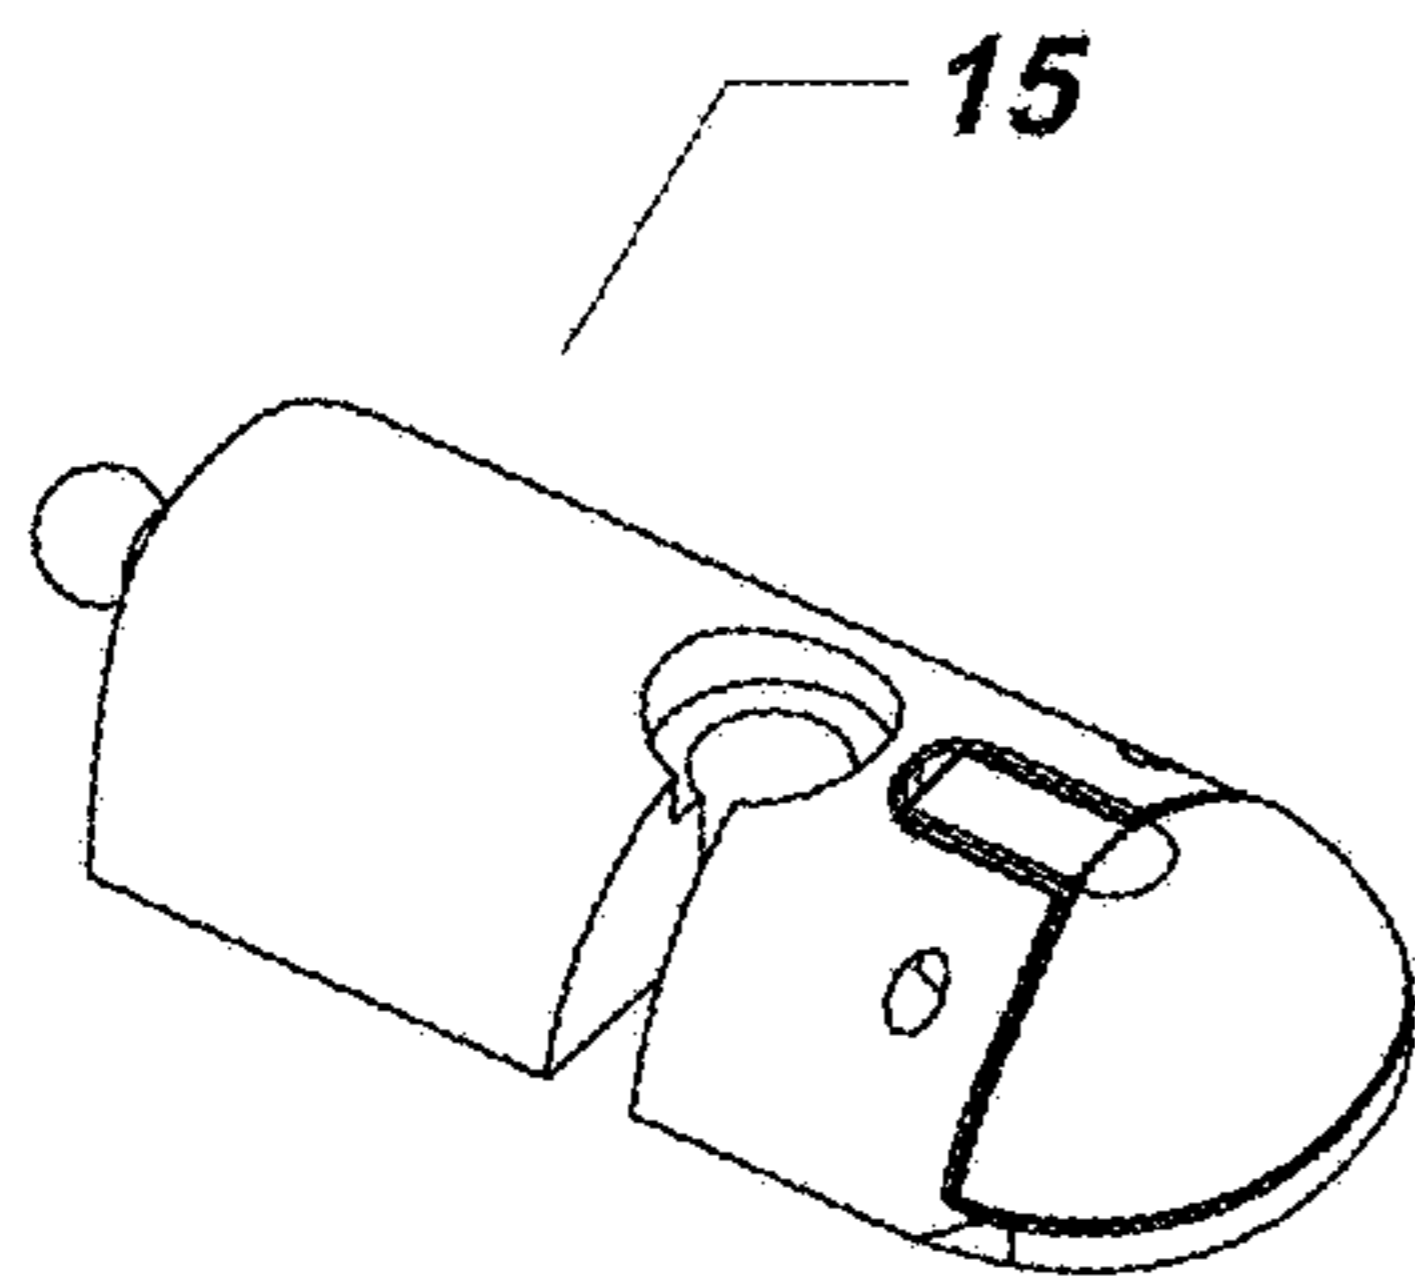


Fig. 35

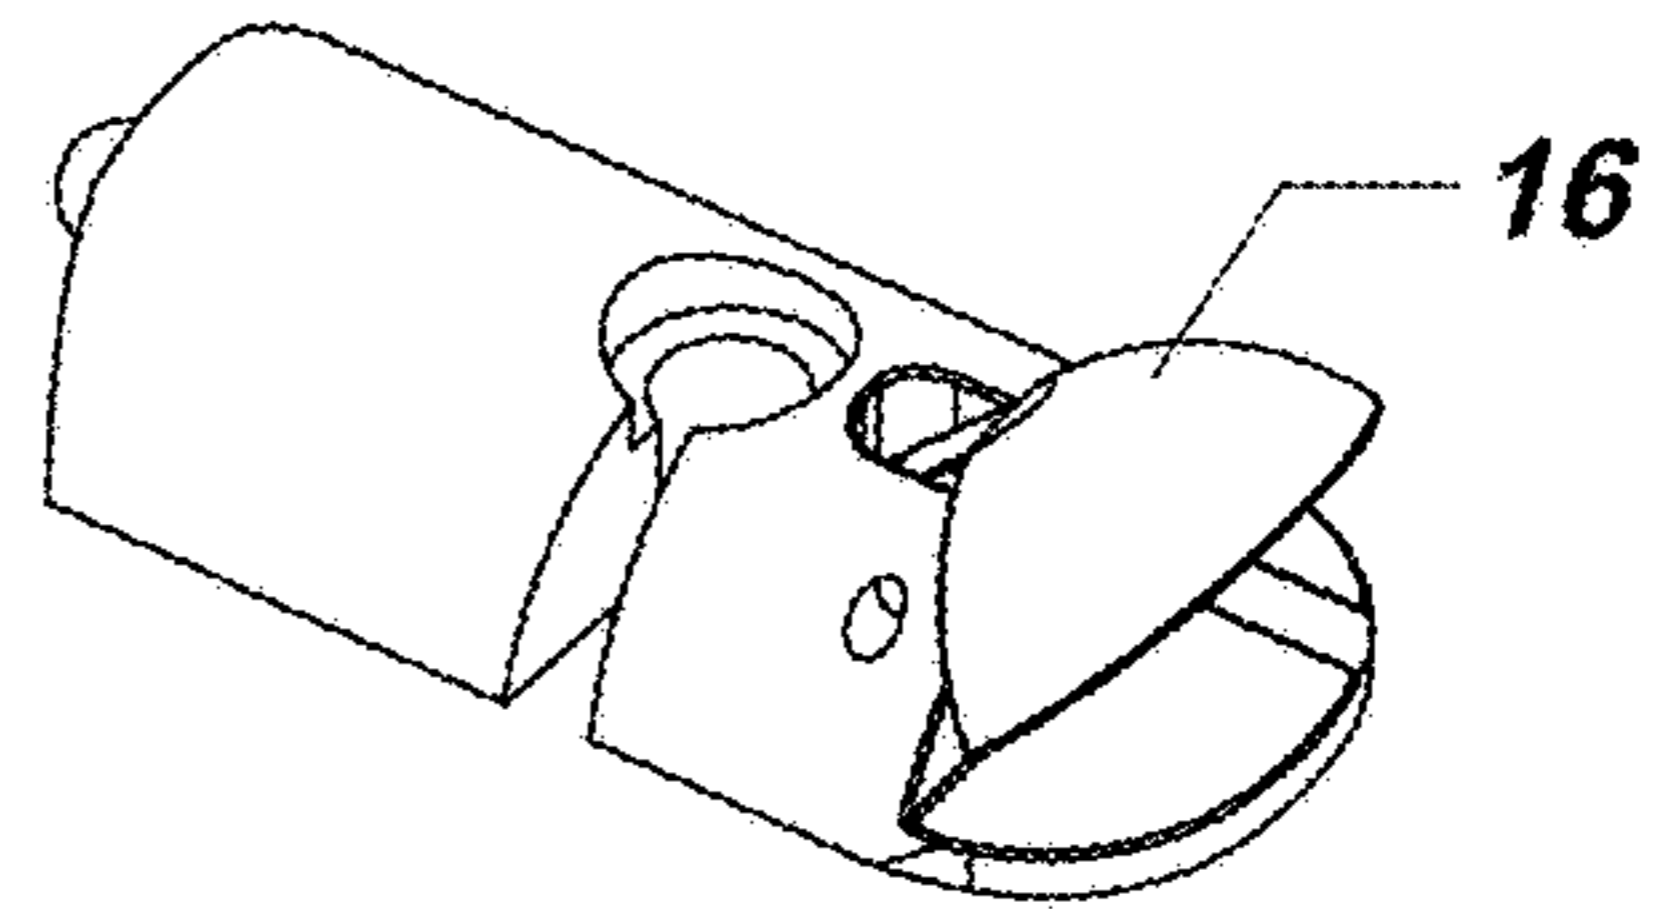


Fig. 36

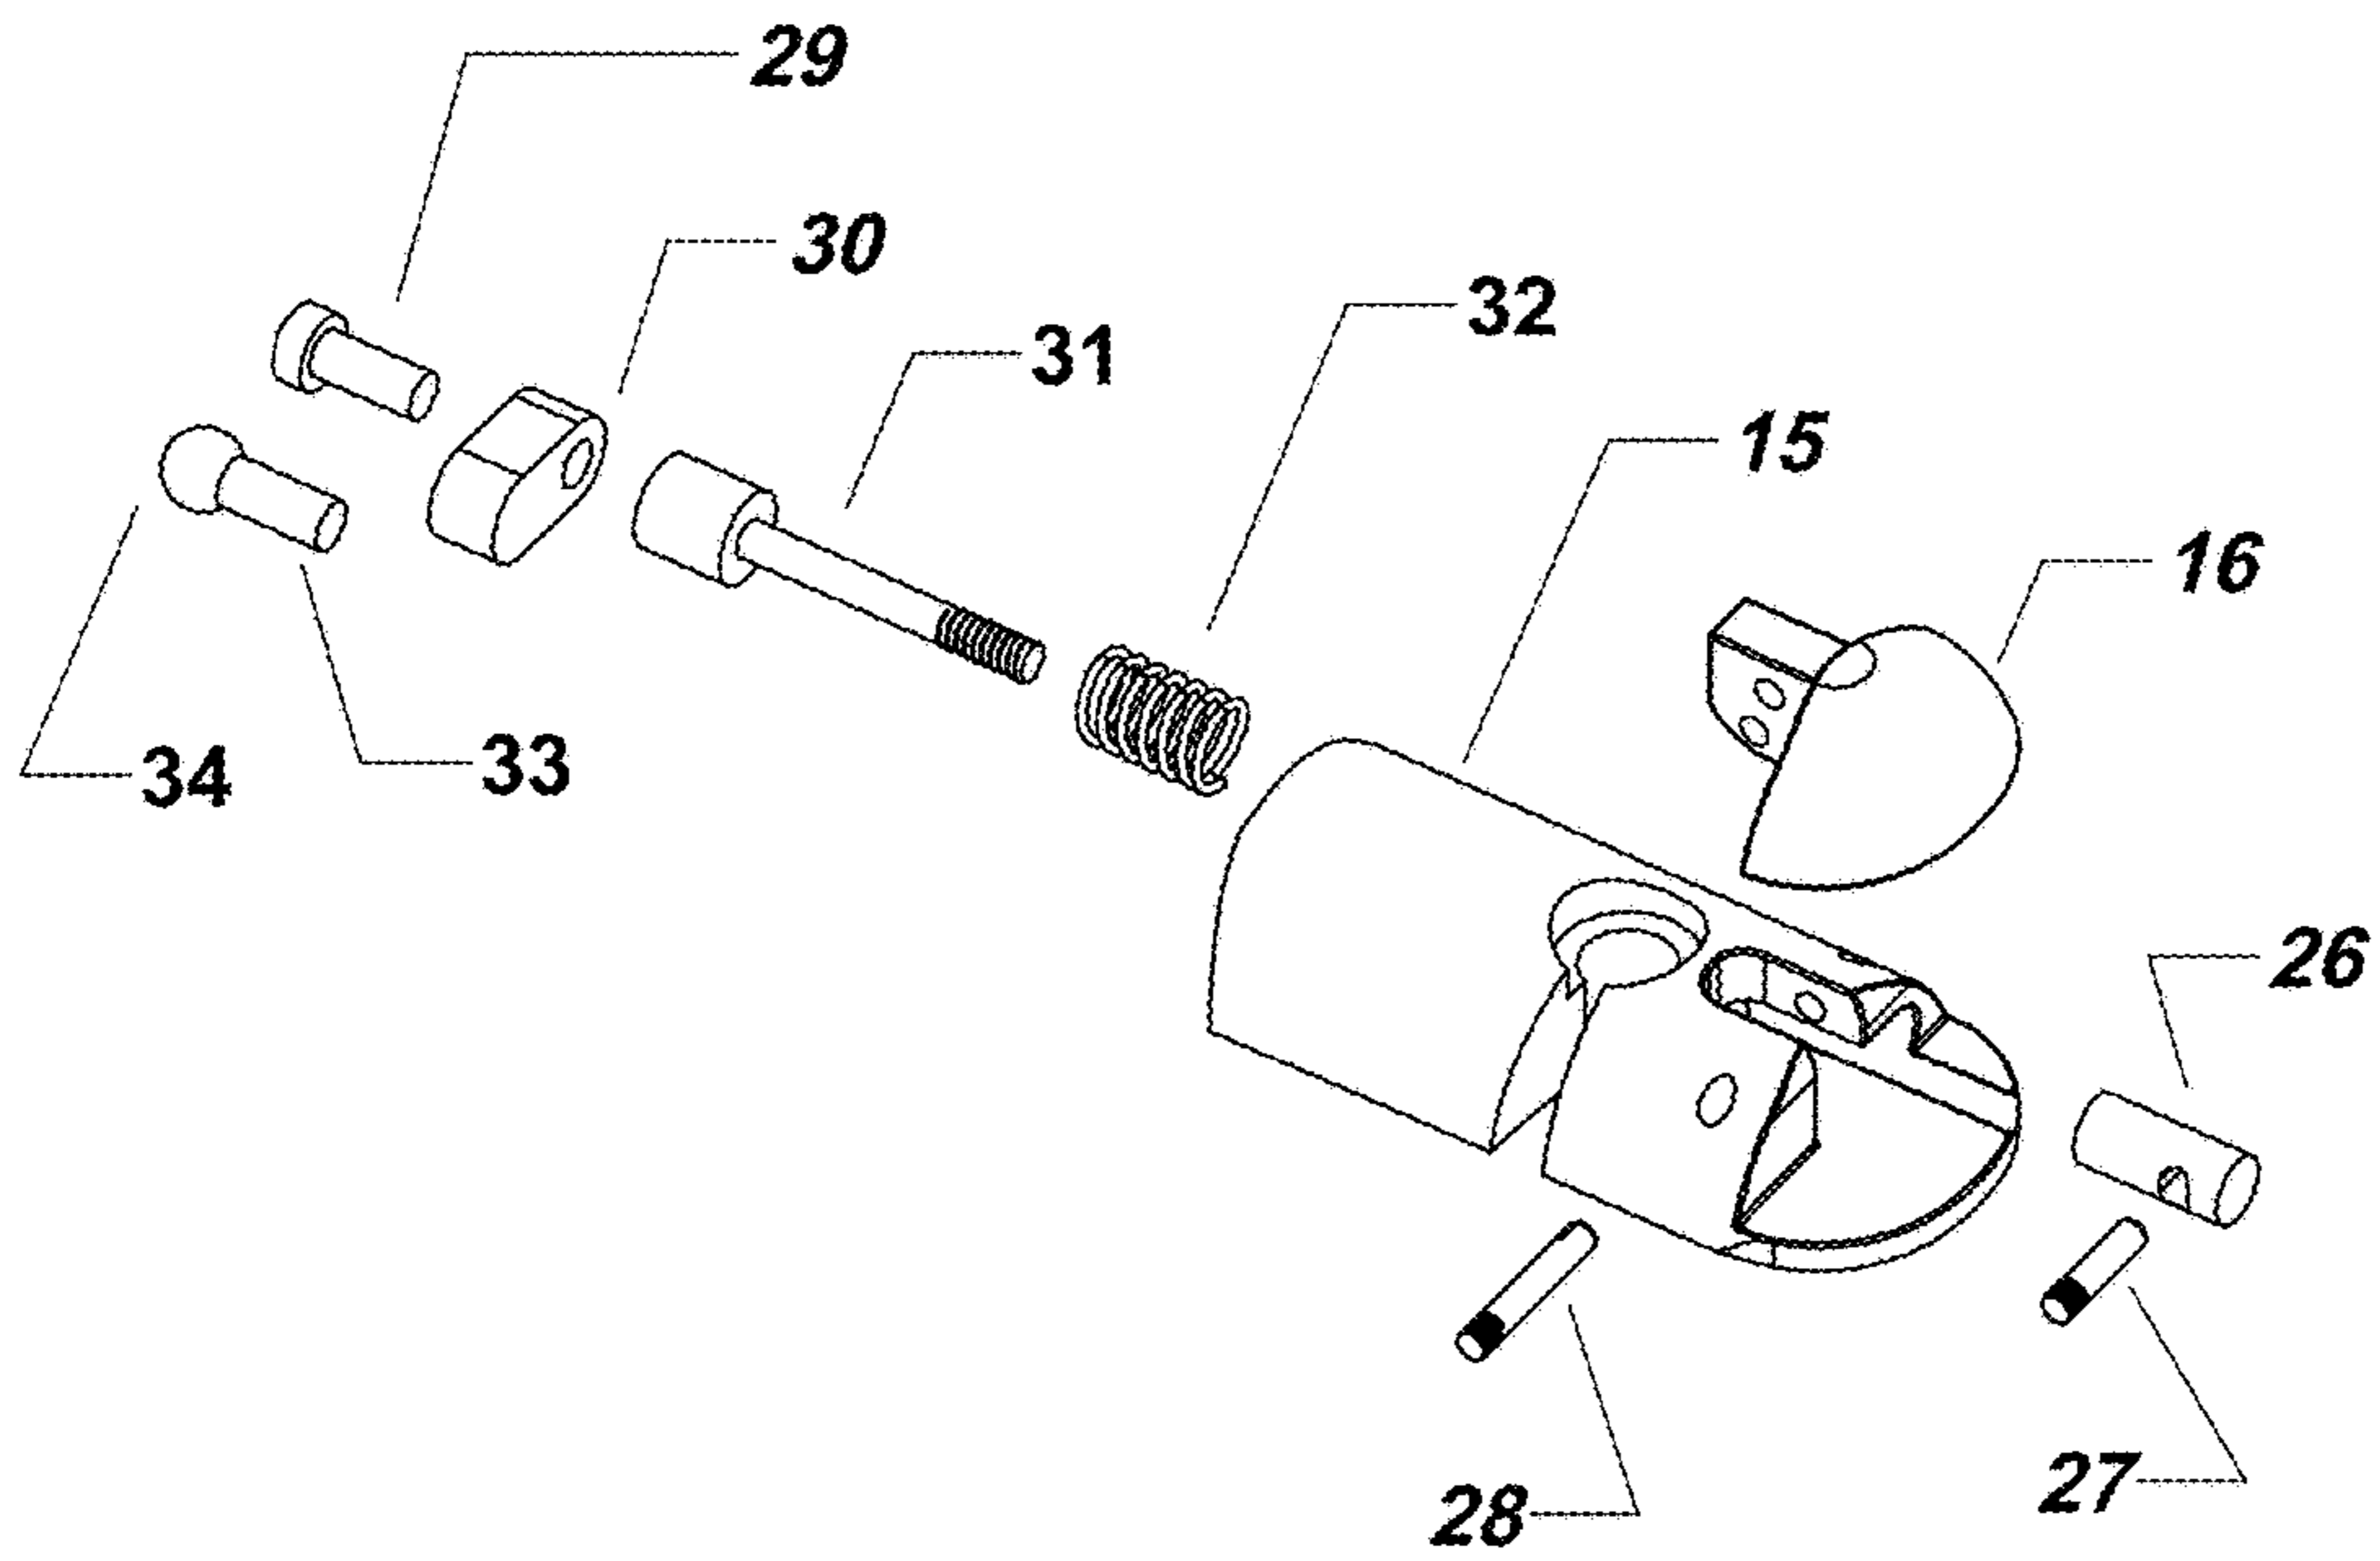


Fig. 37

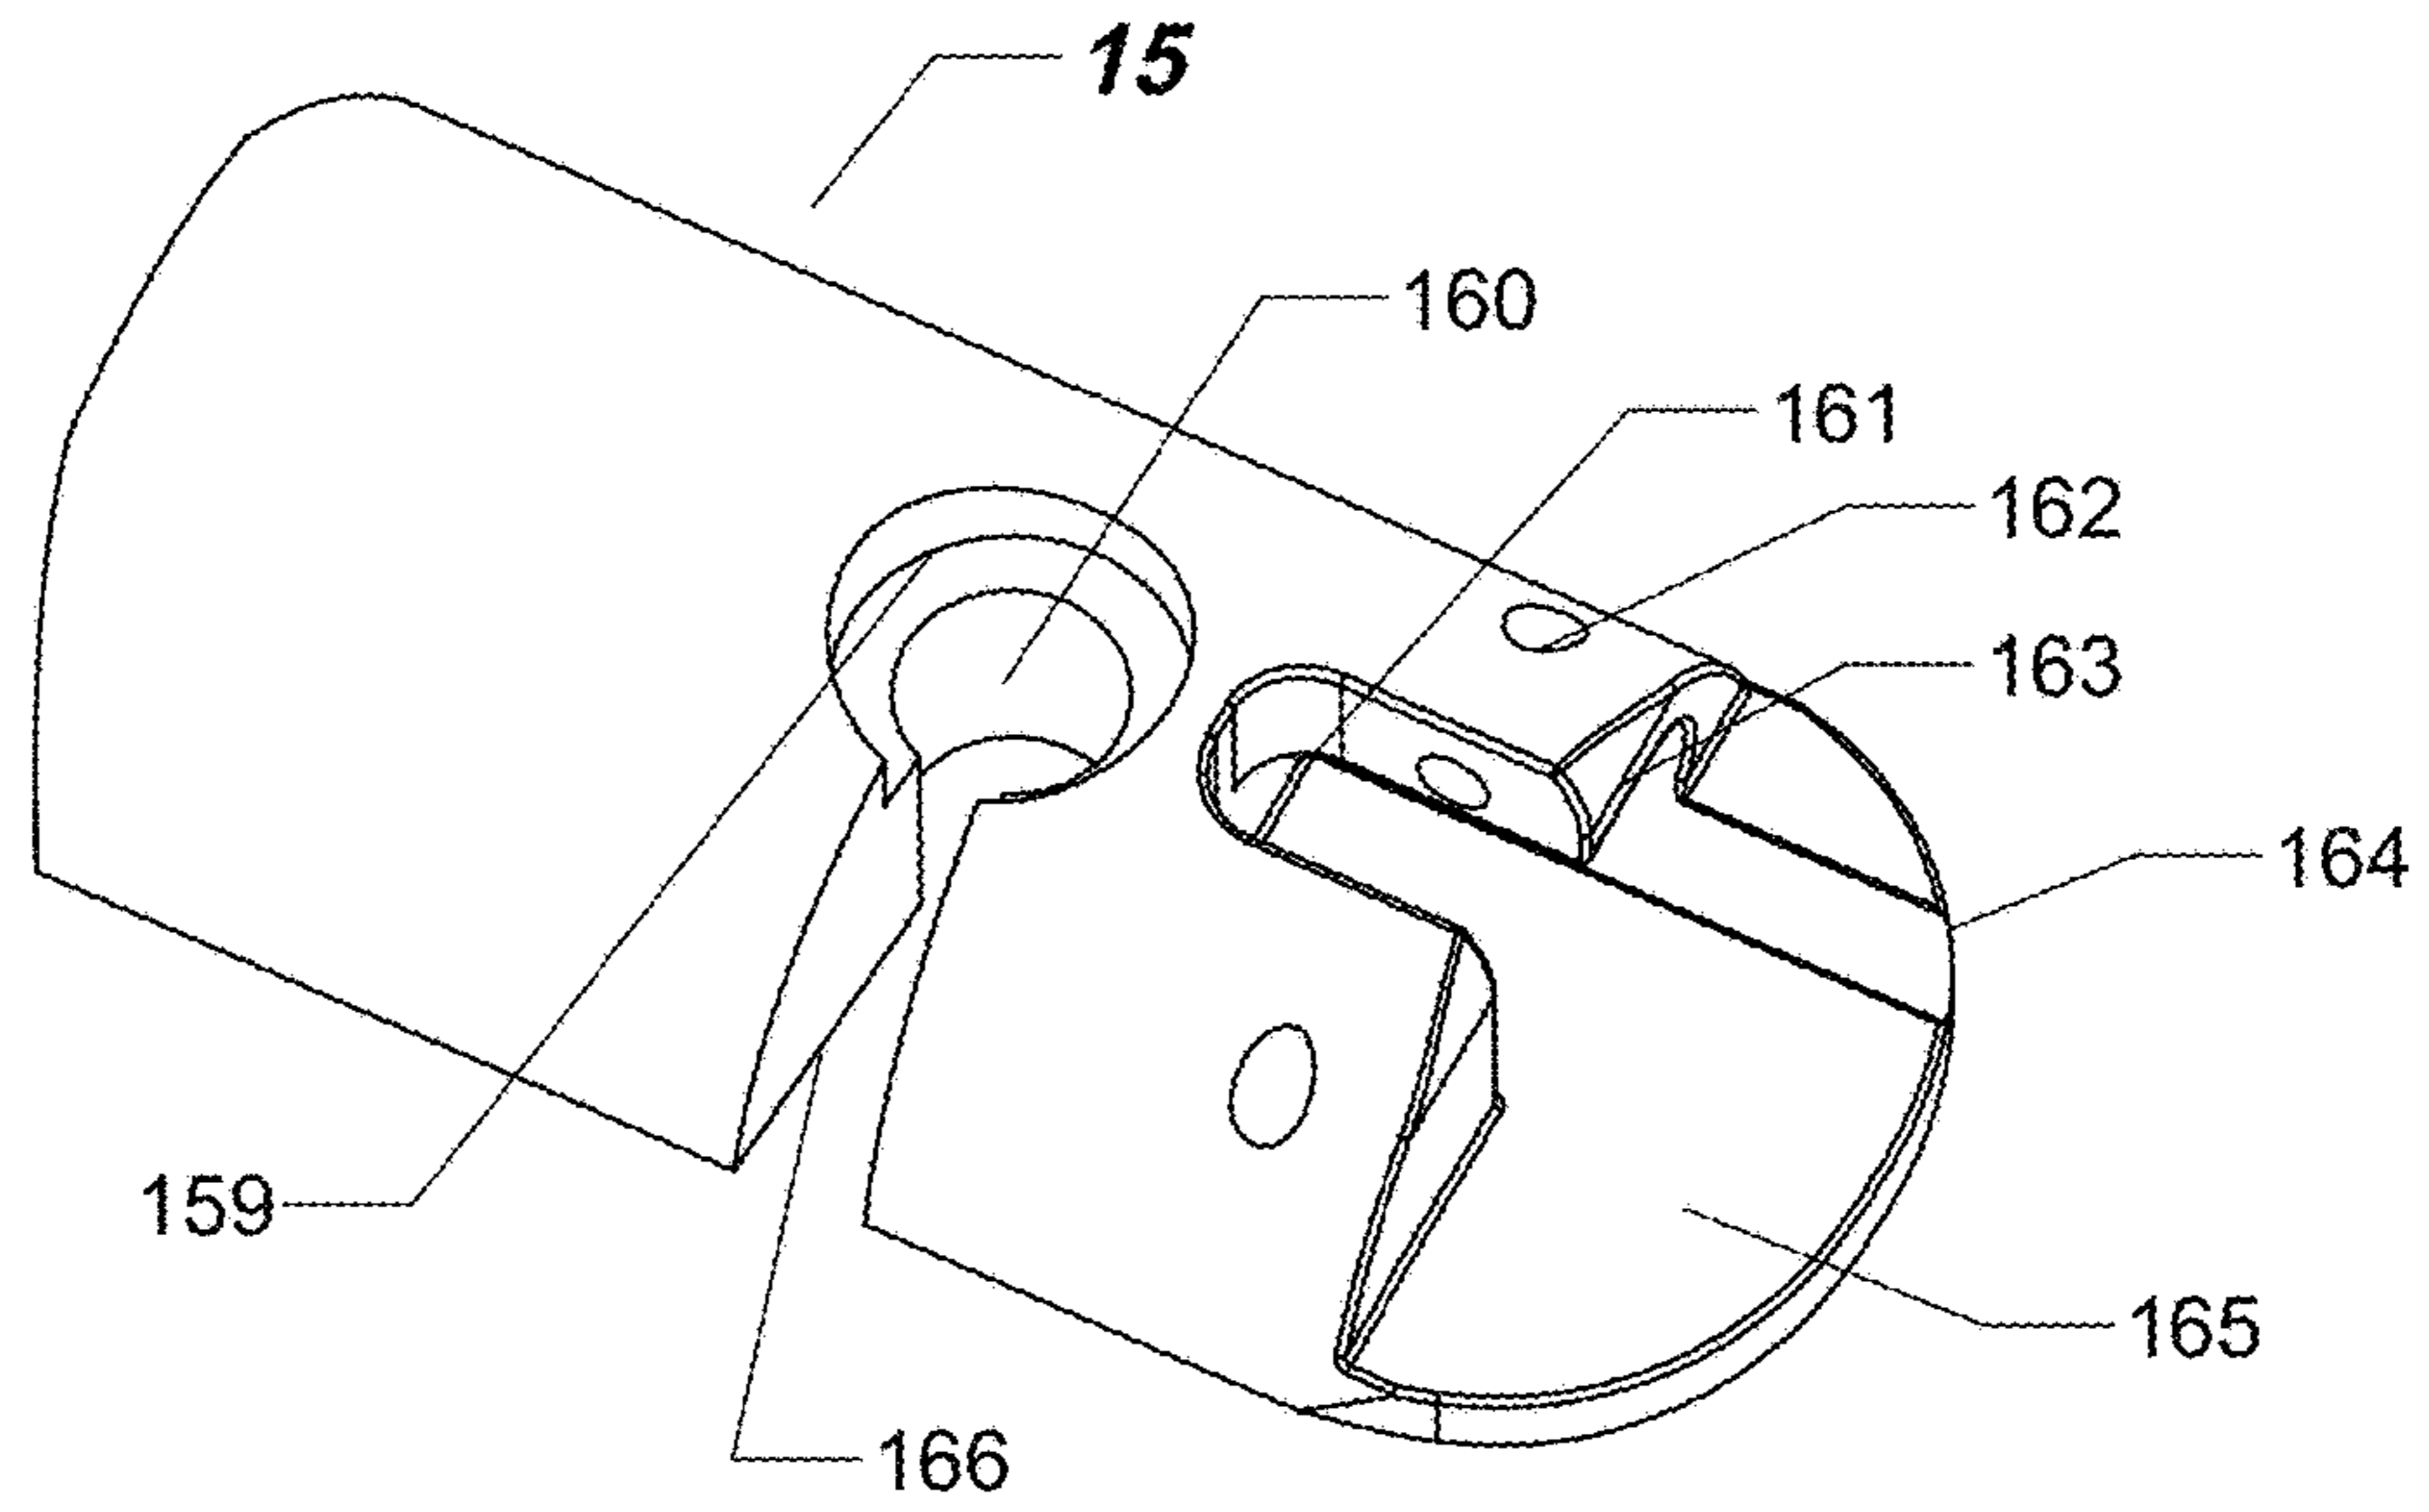


Fig. 38

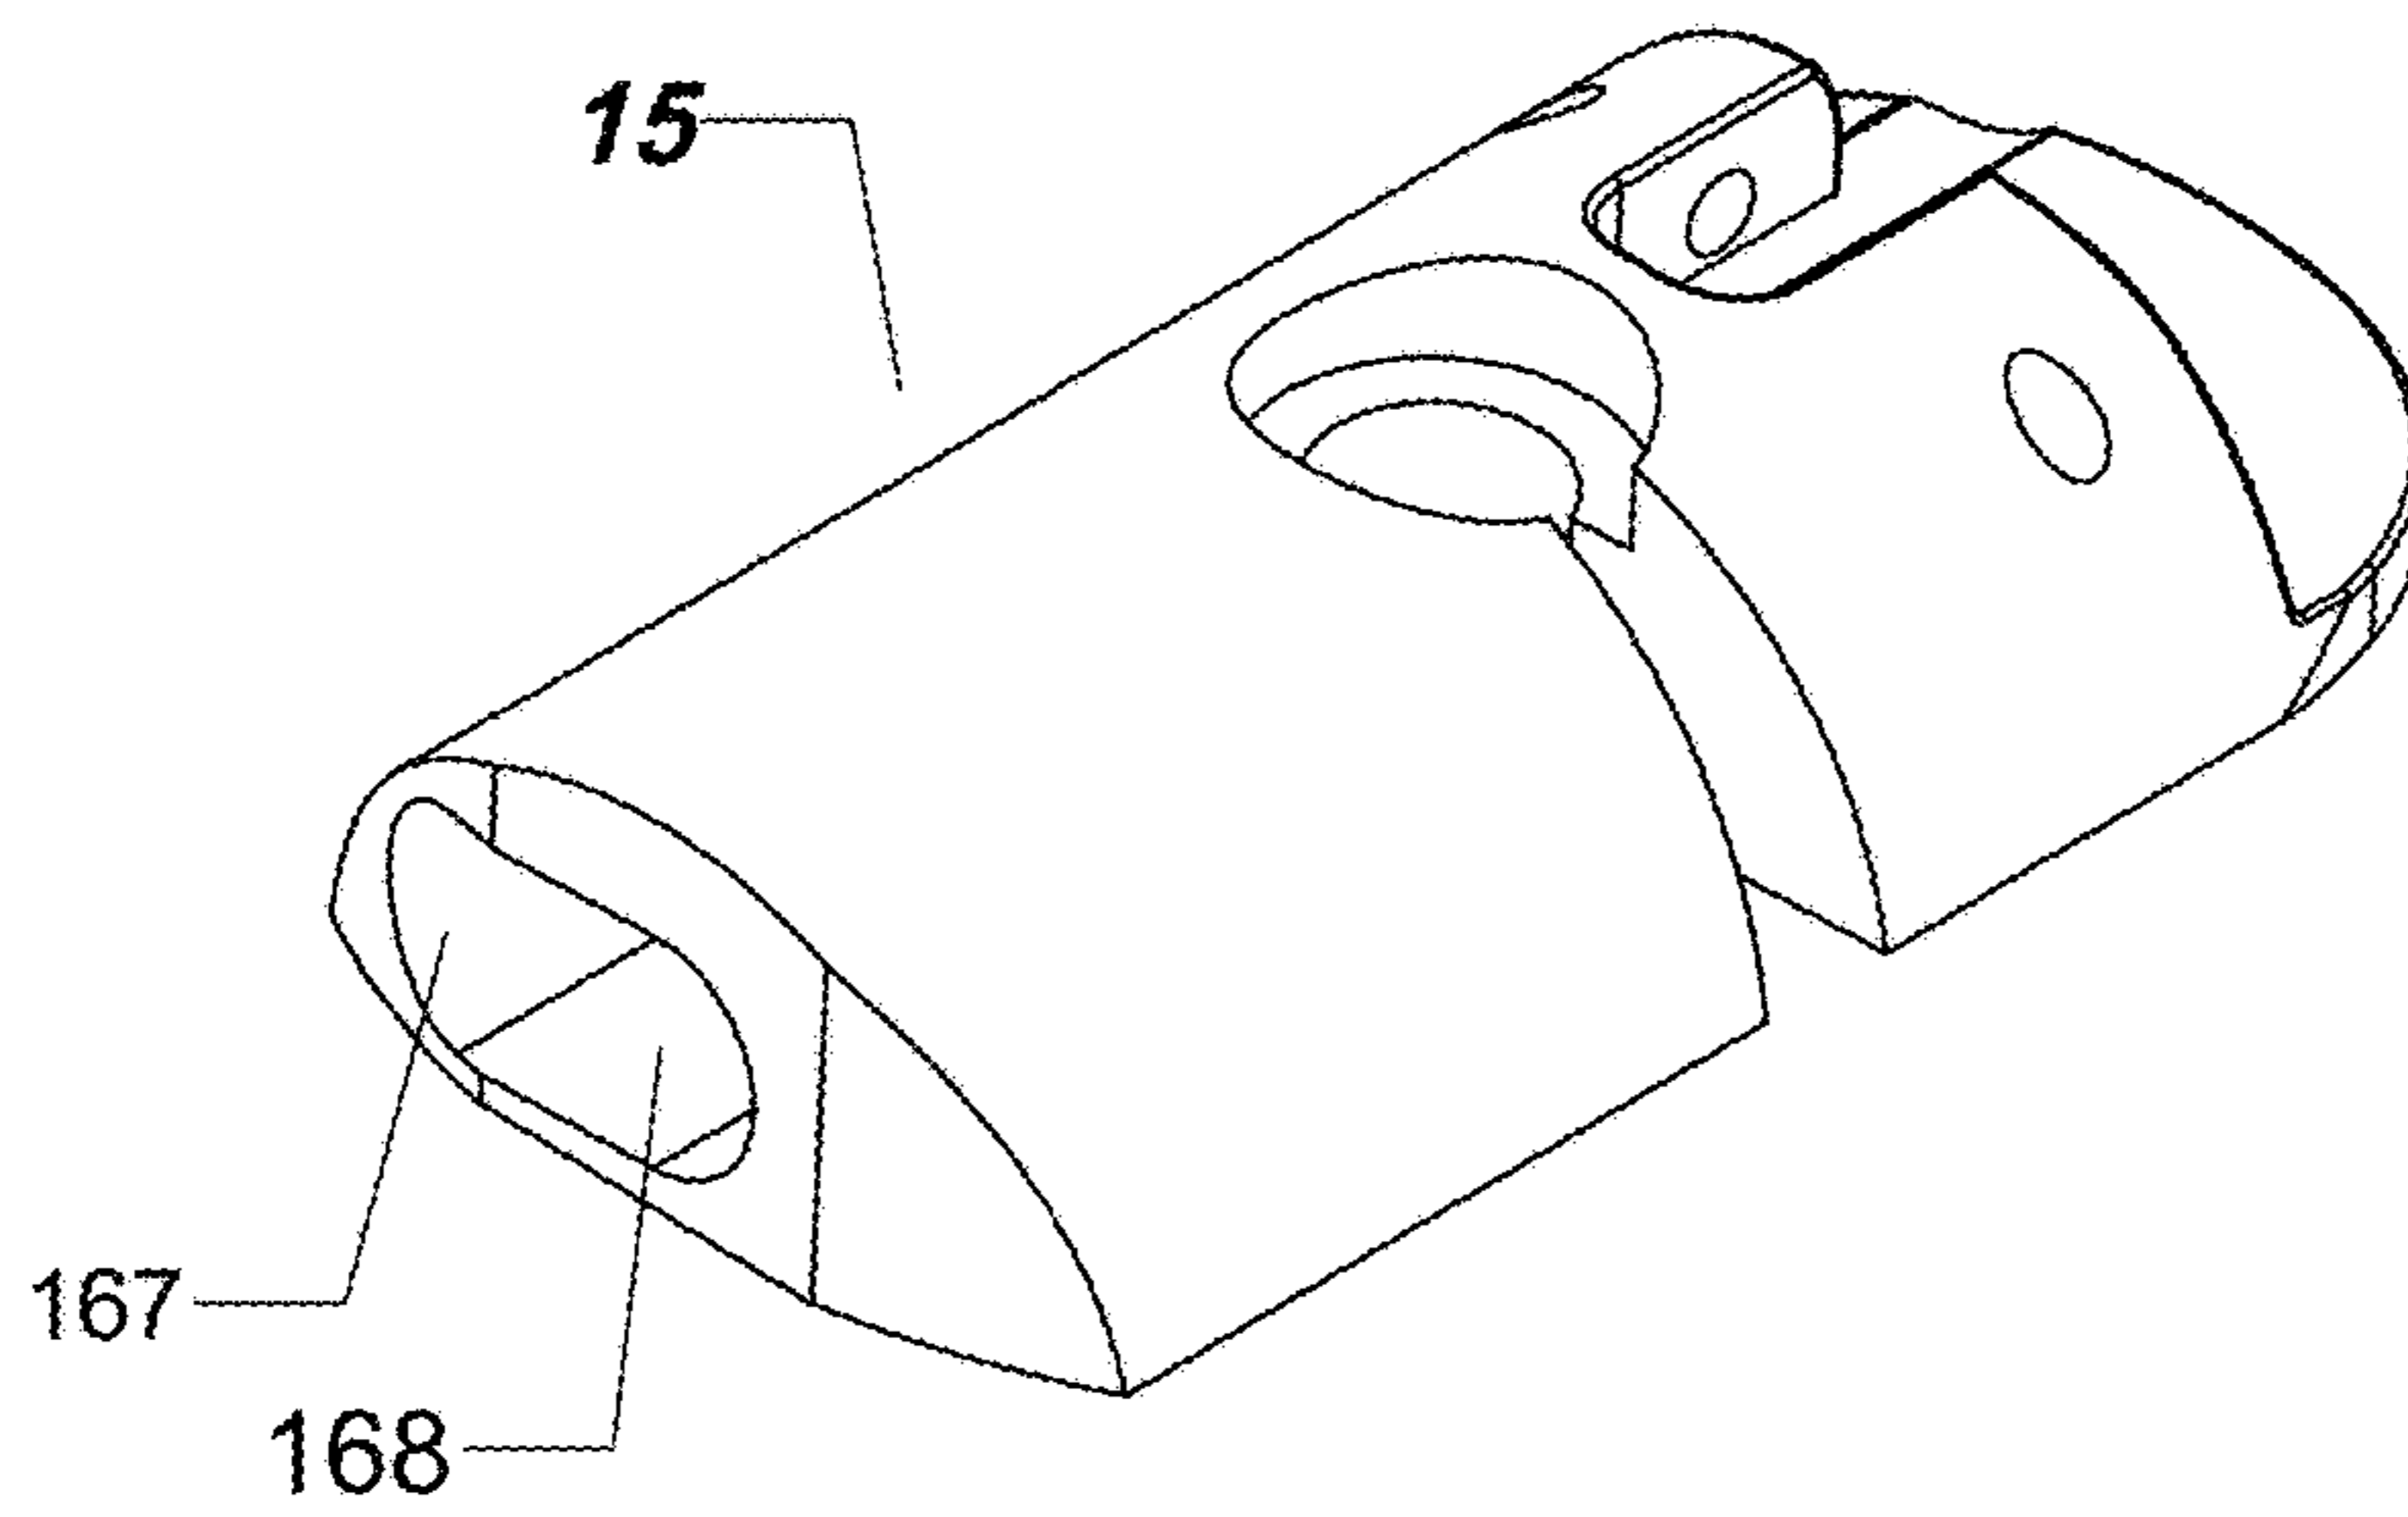


Fig. 39

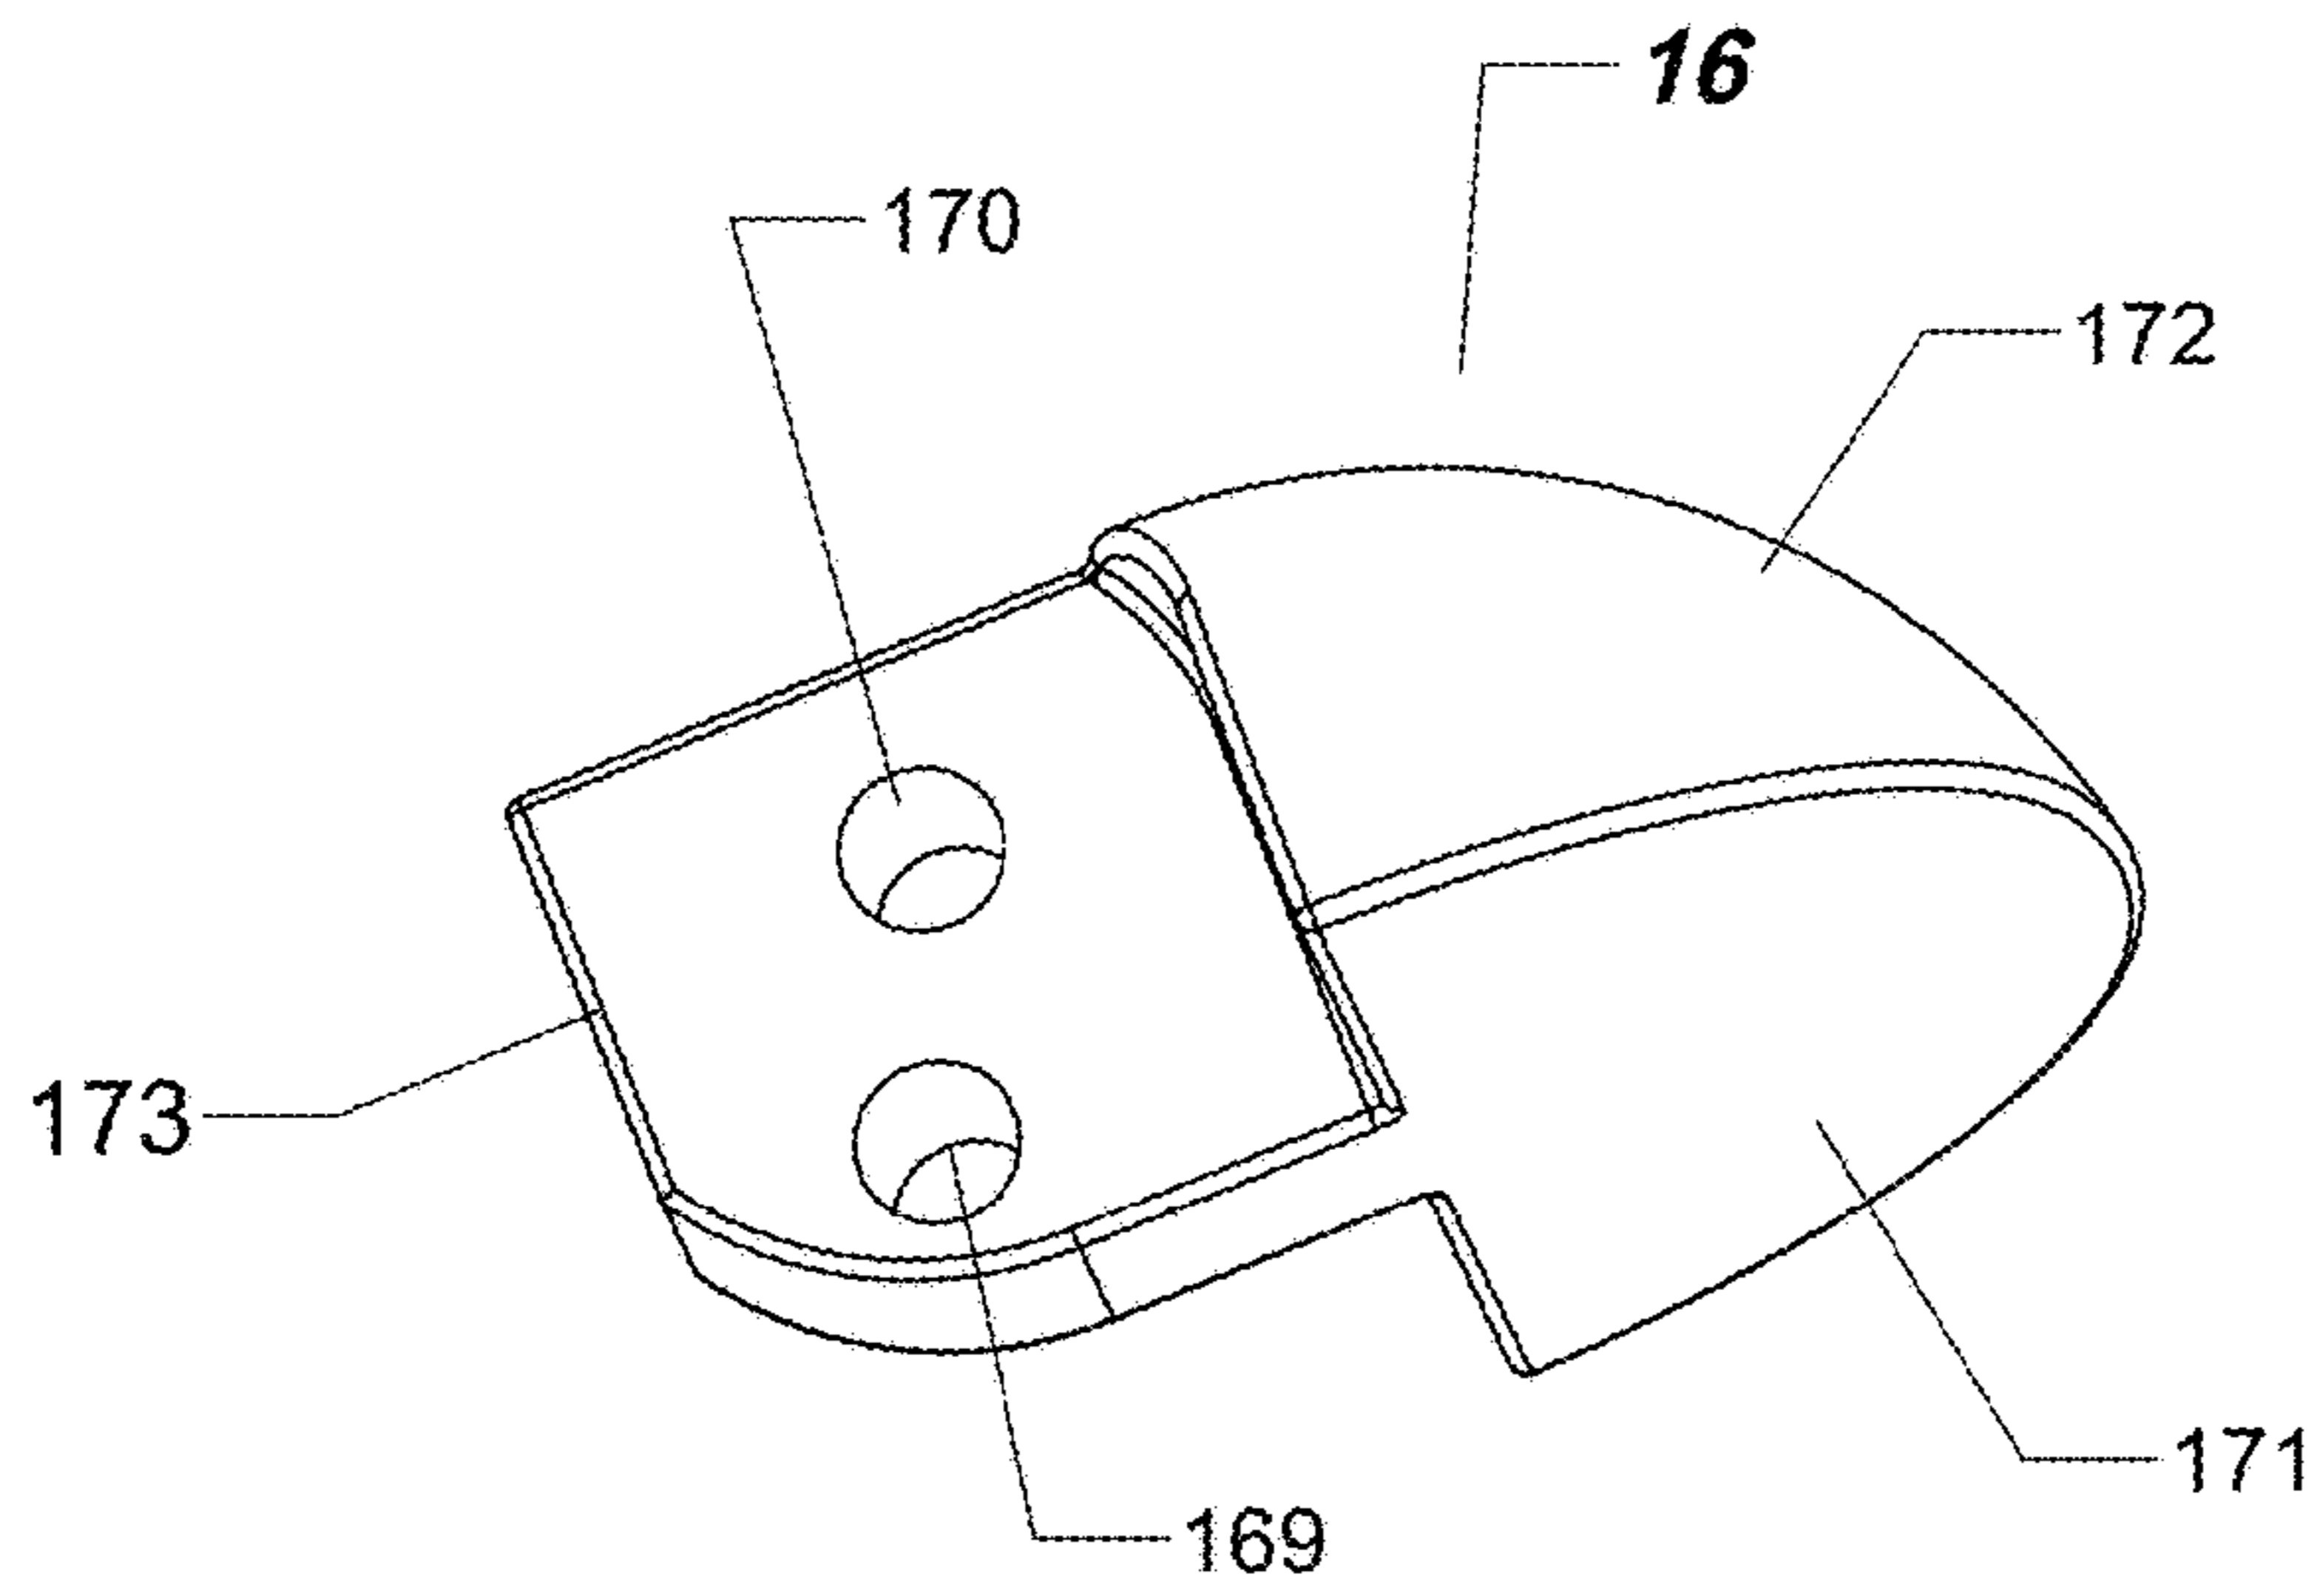


Fig. 40

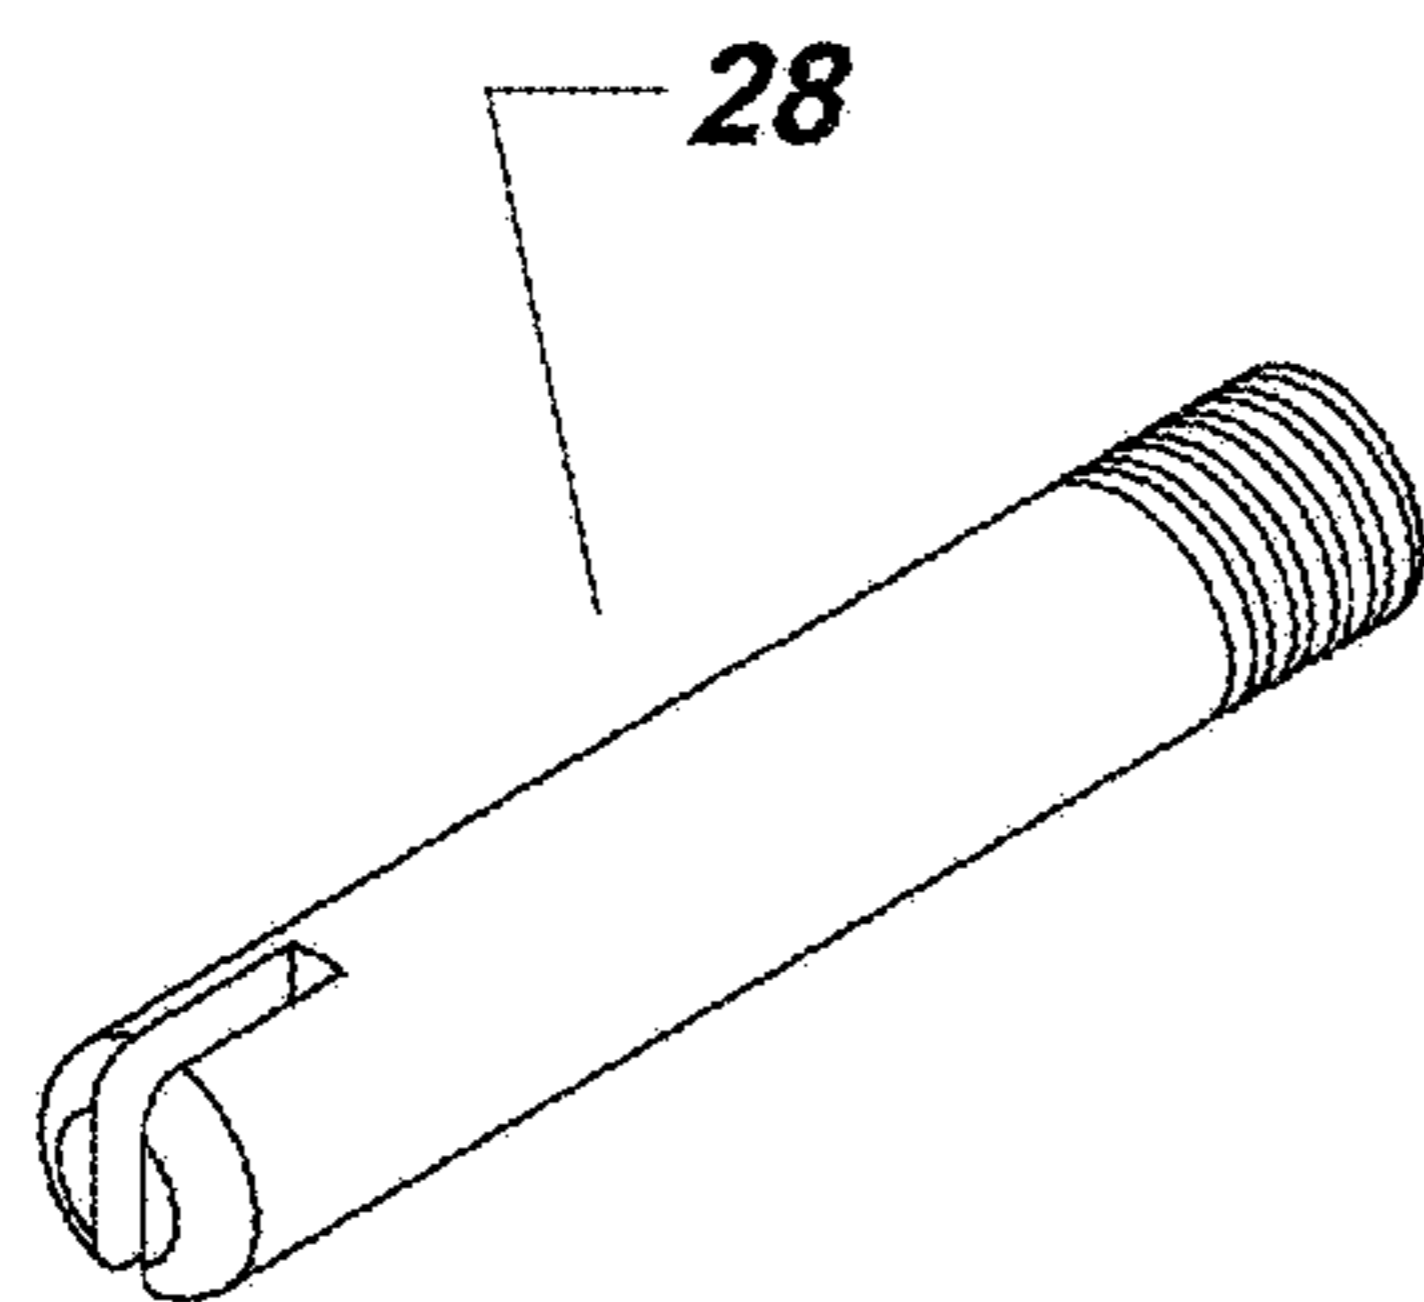


Fig. 41

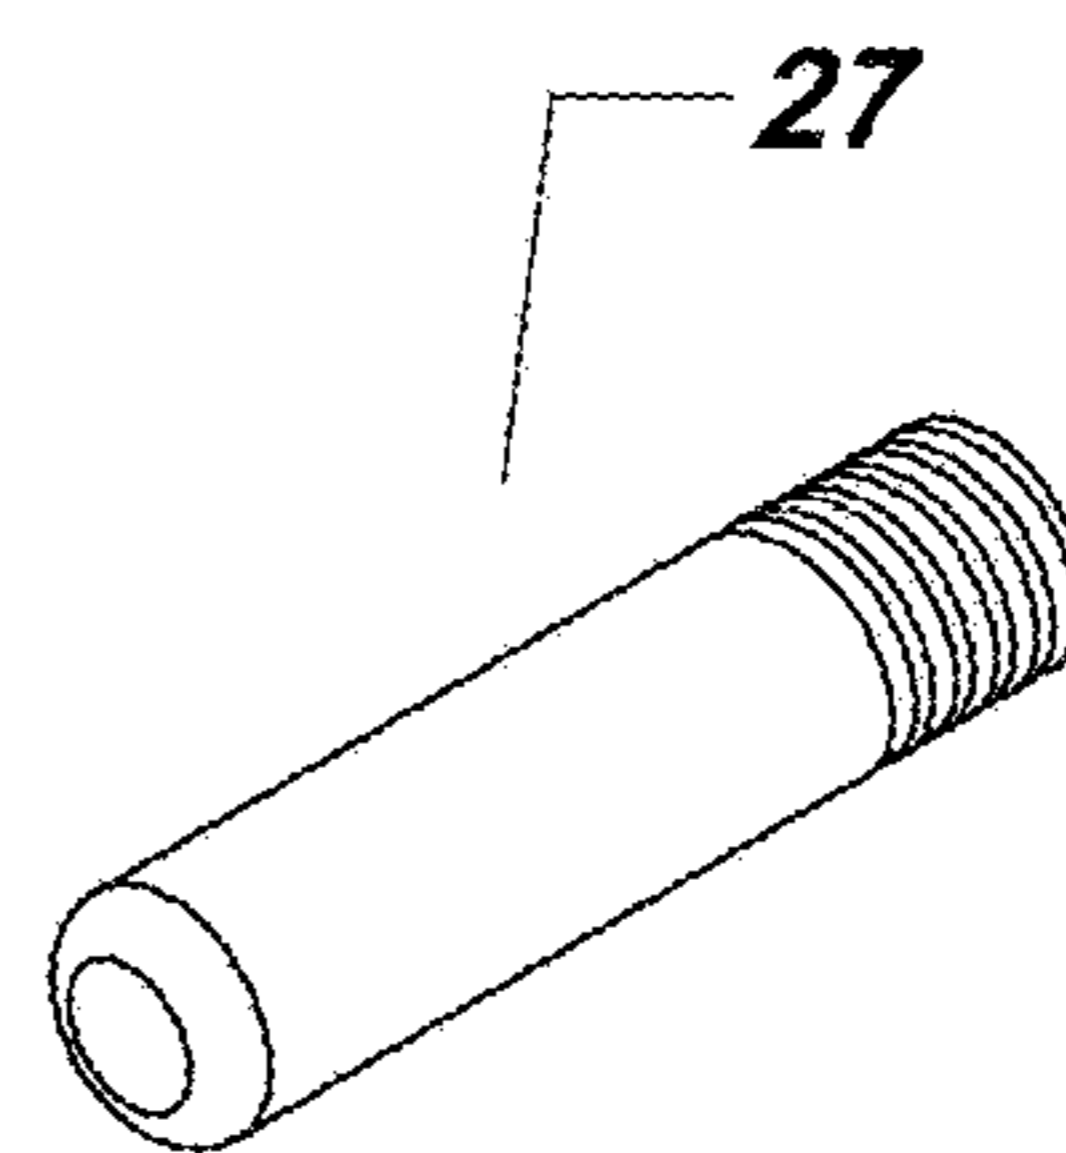


Fig. 42

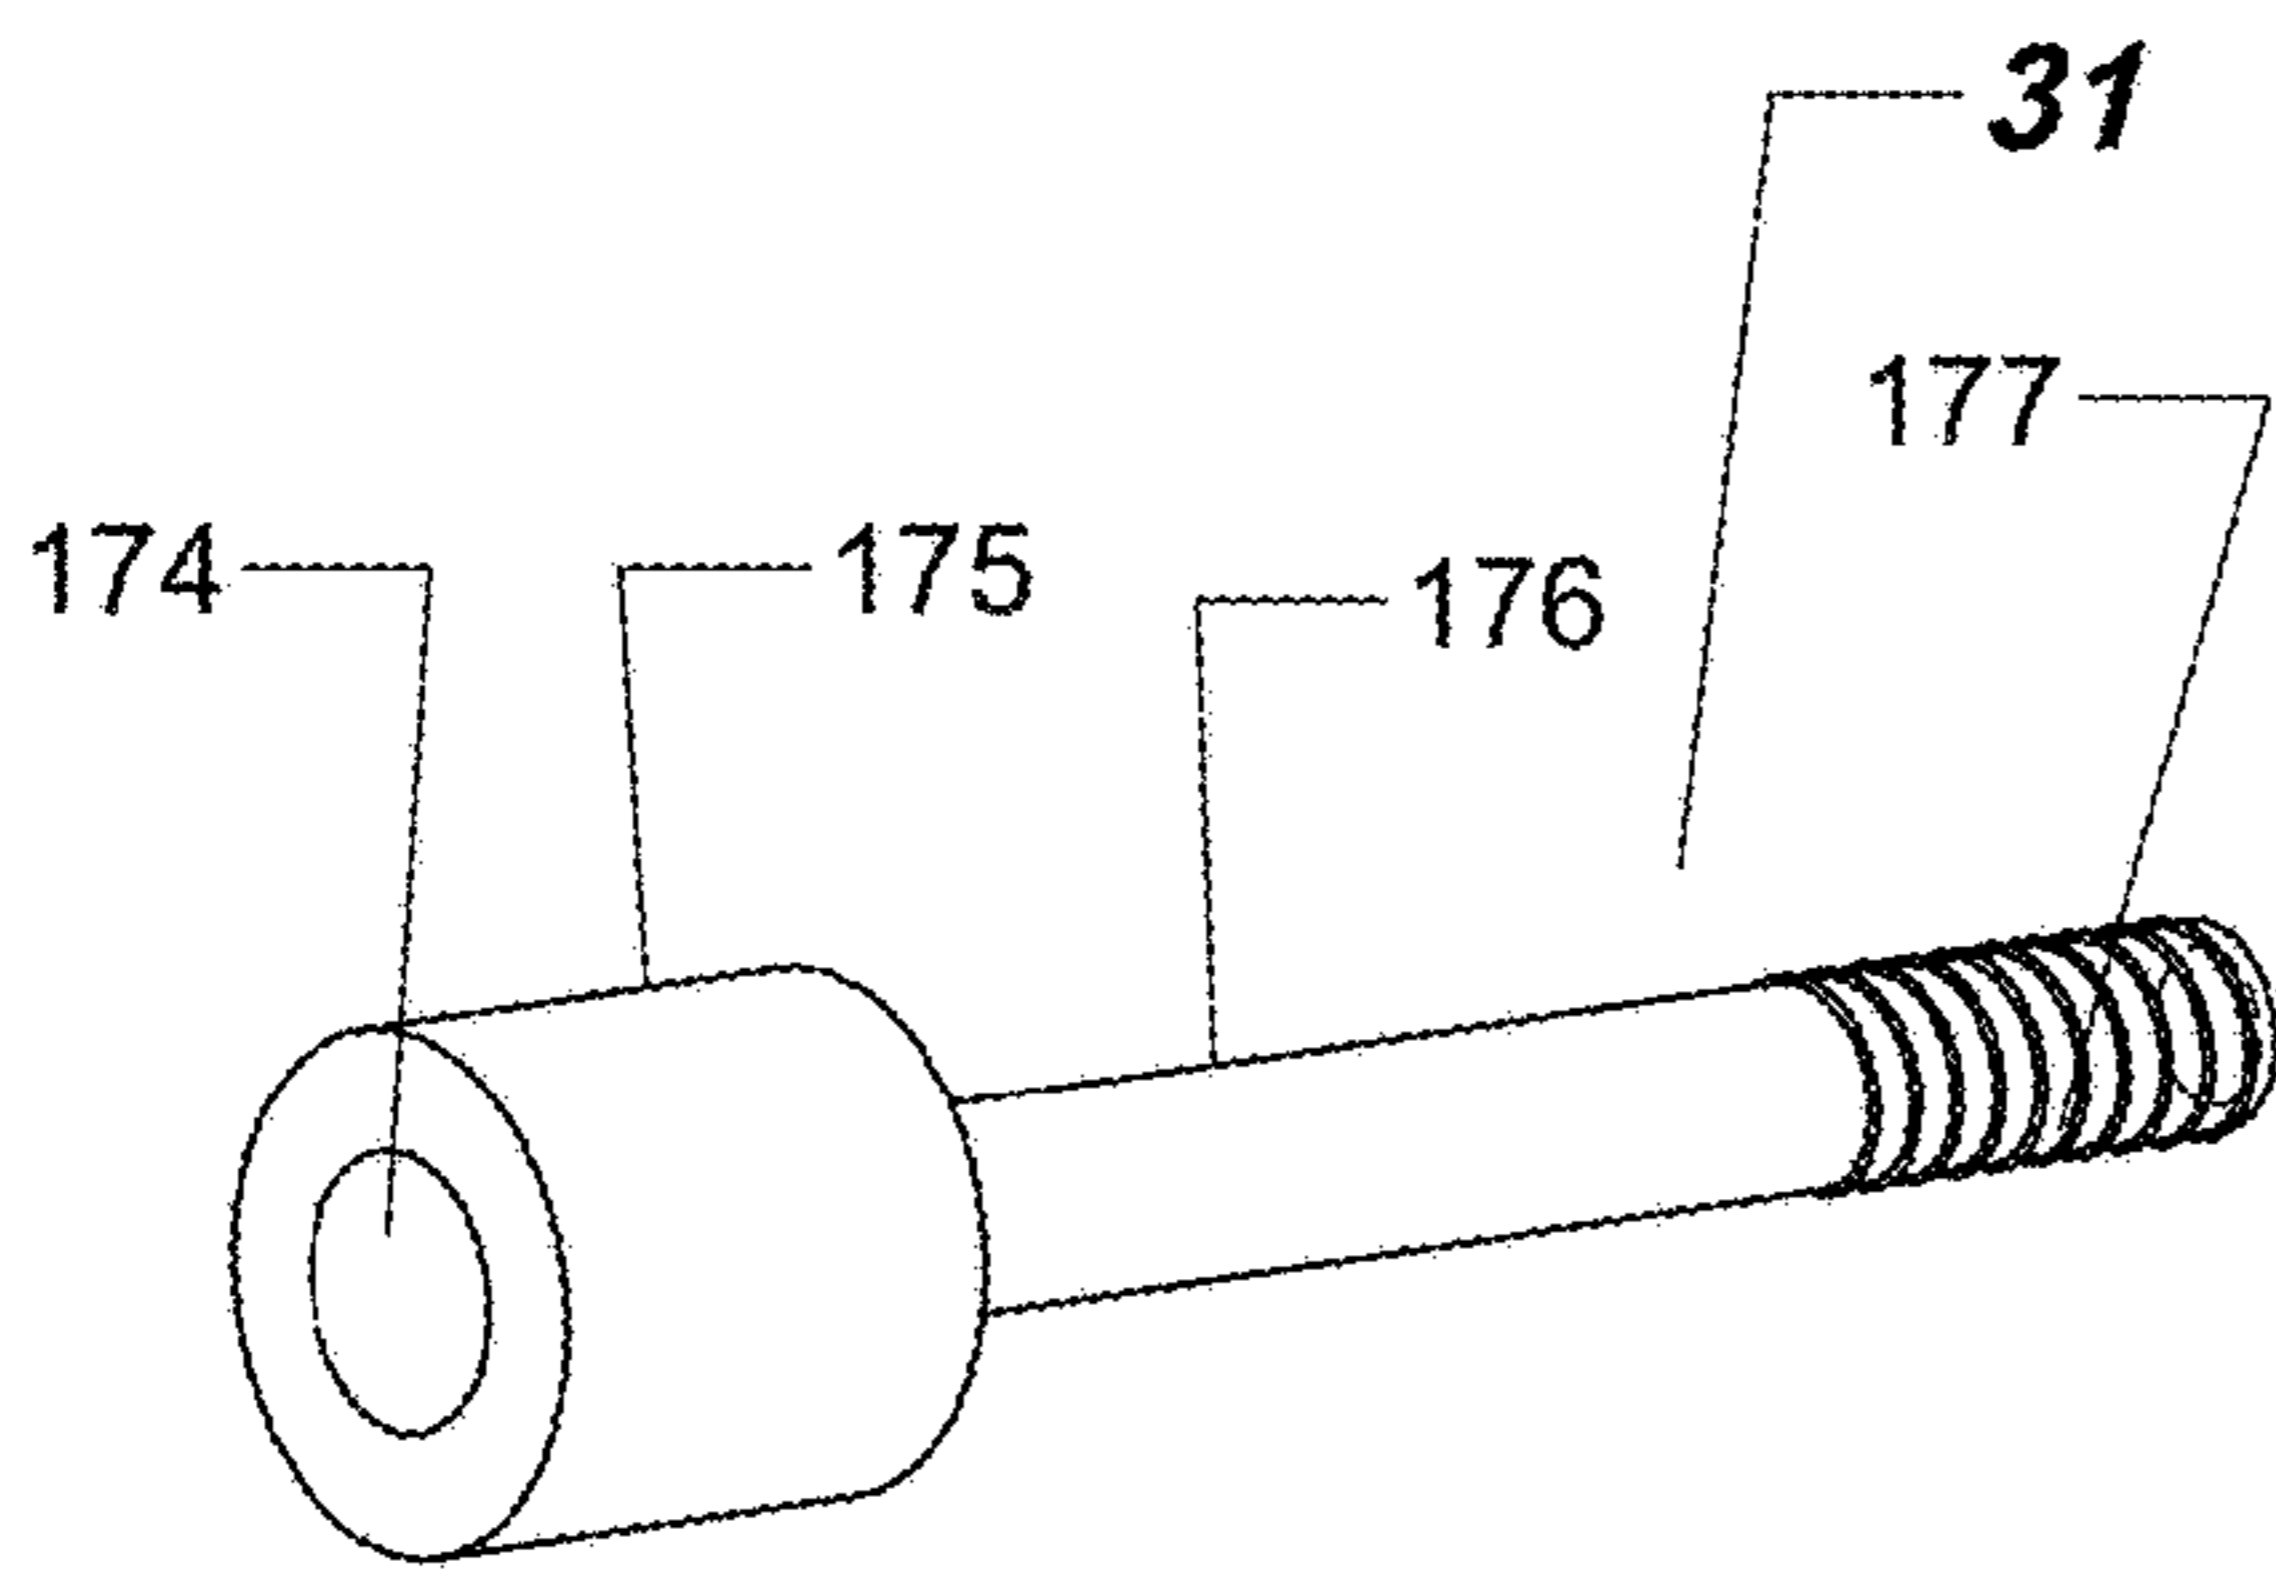


Fig. 43

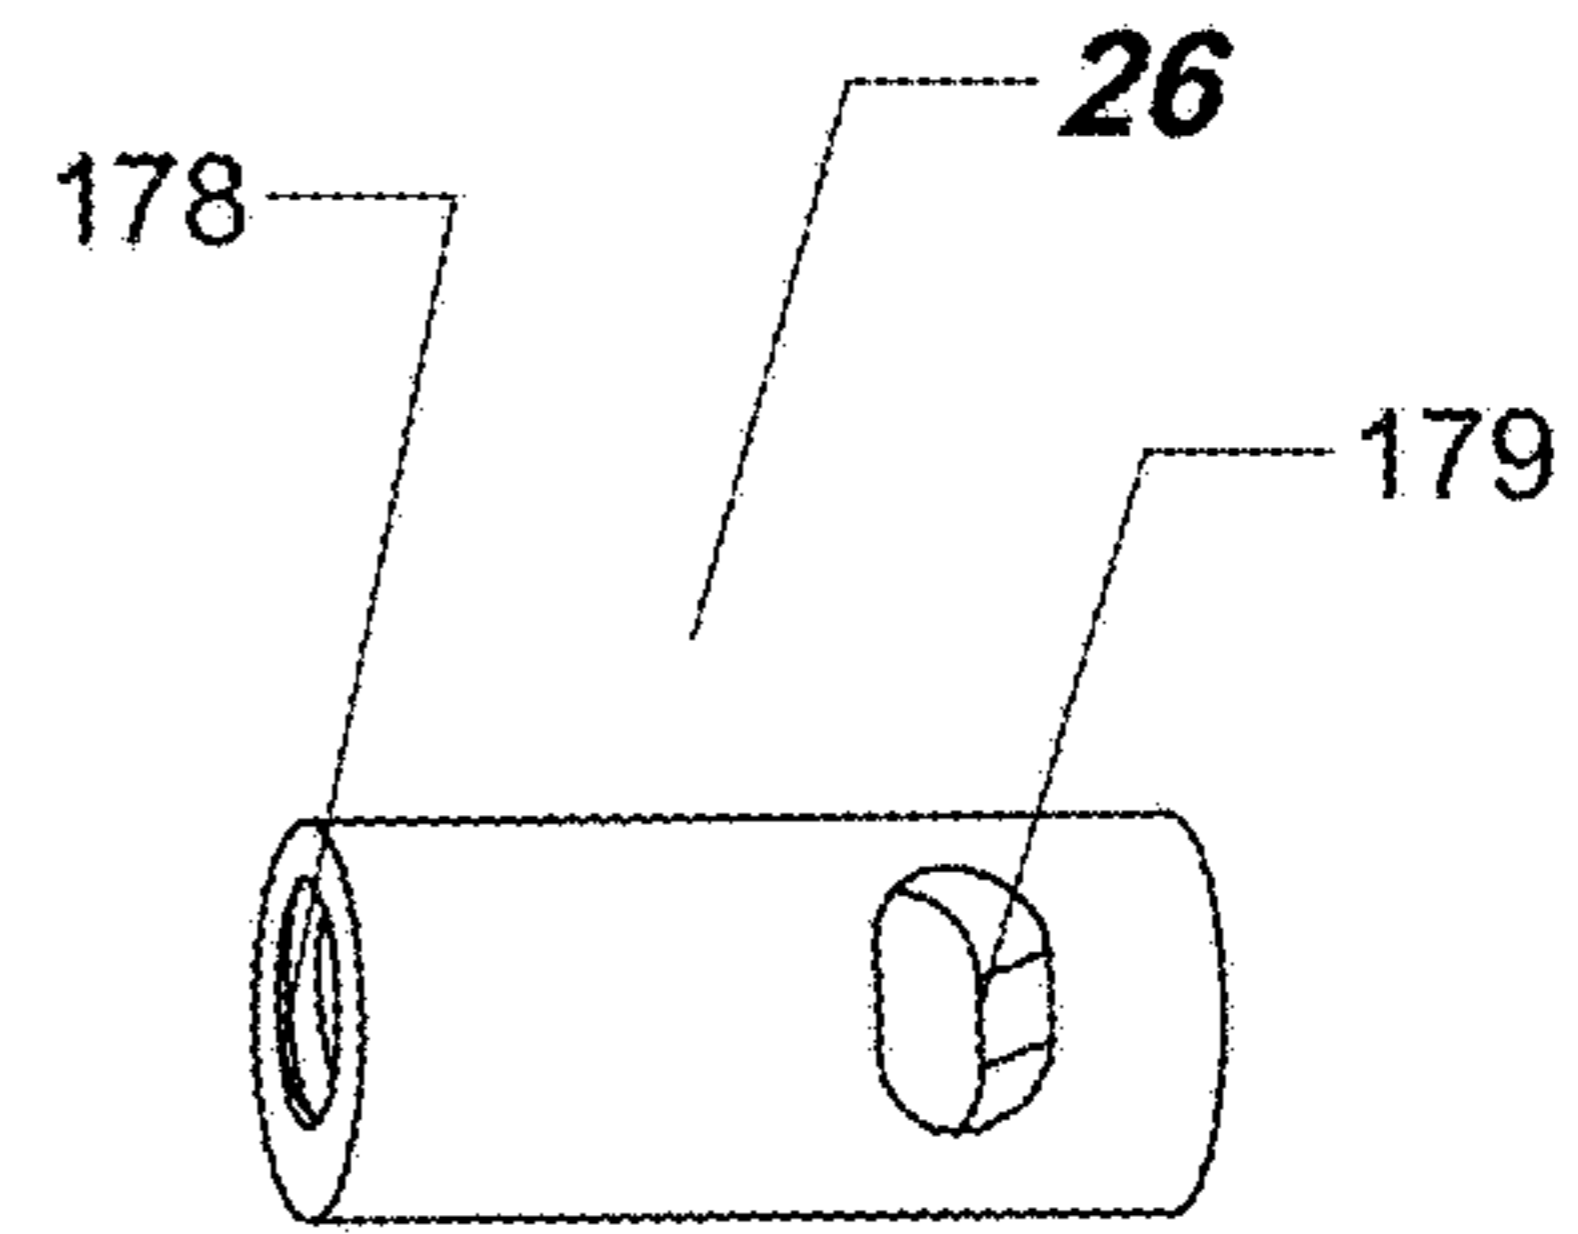


Fig. 44

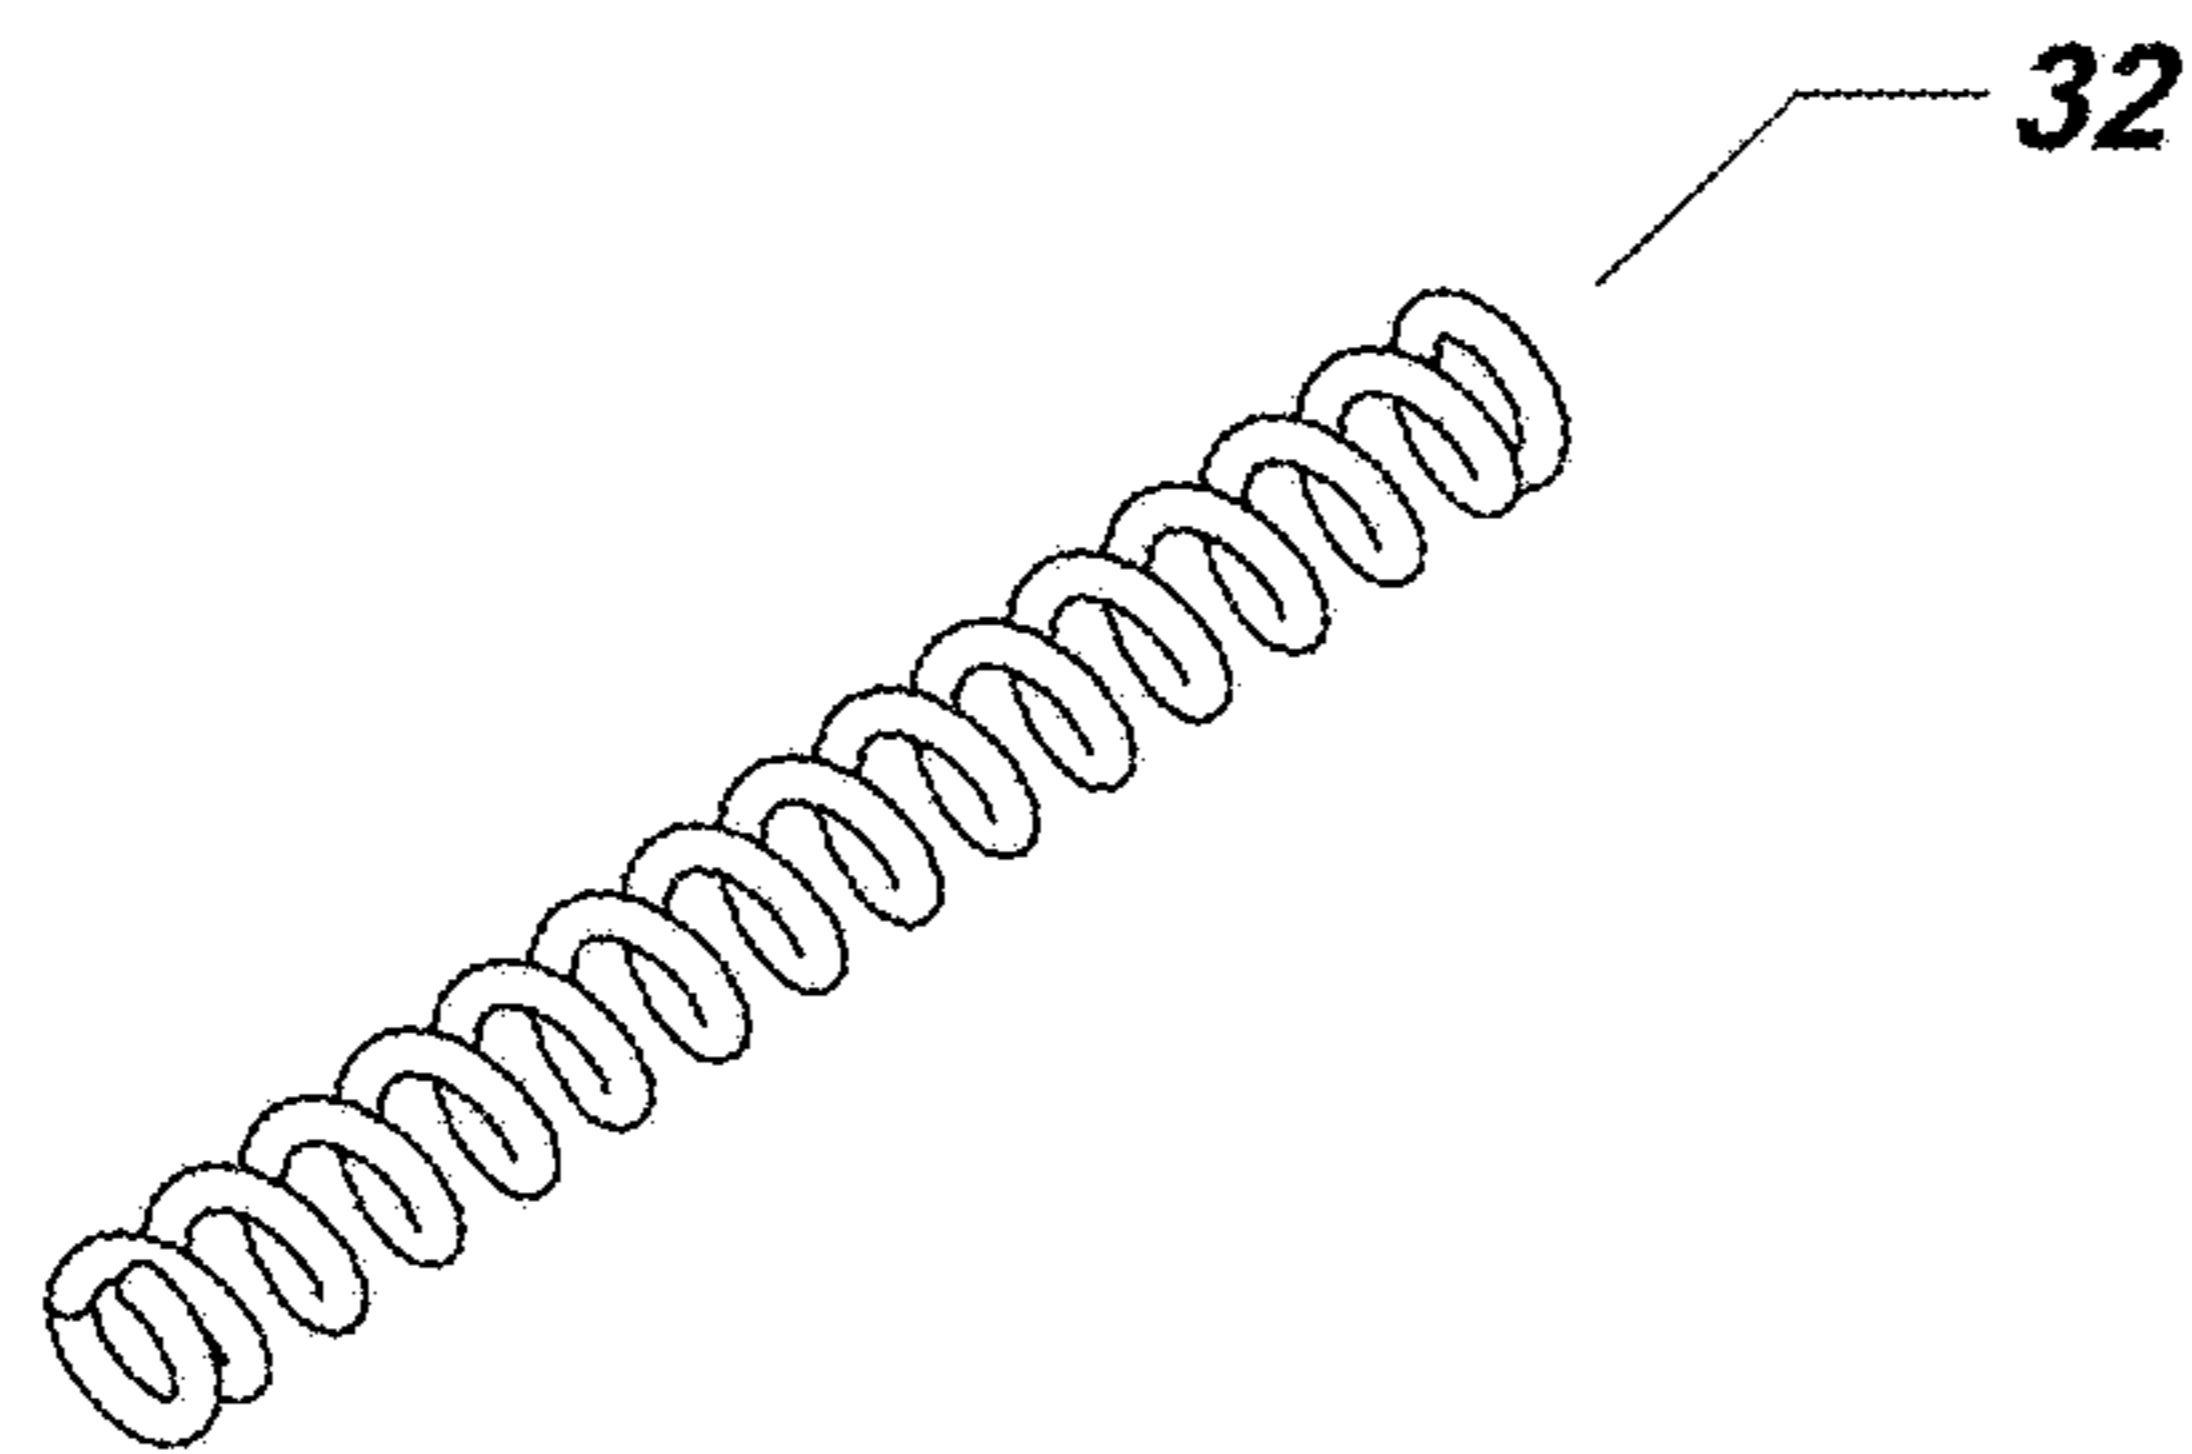


Fig. 45

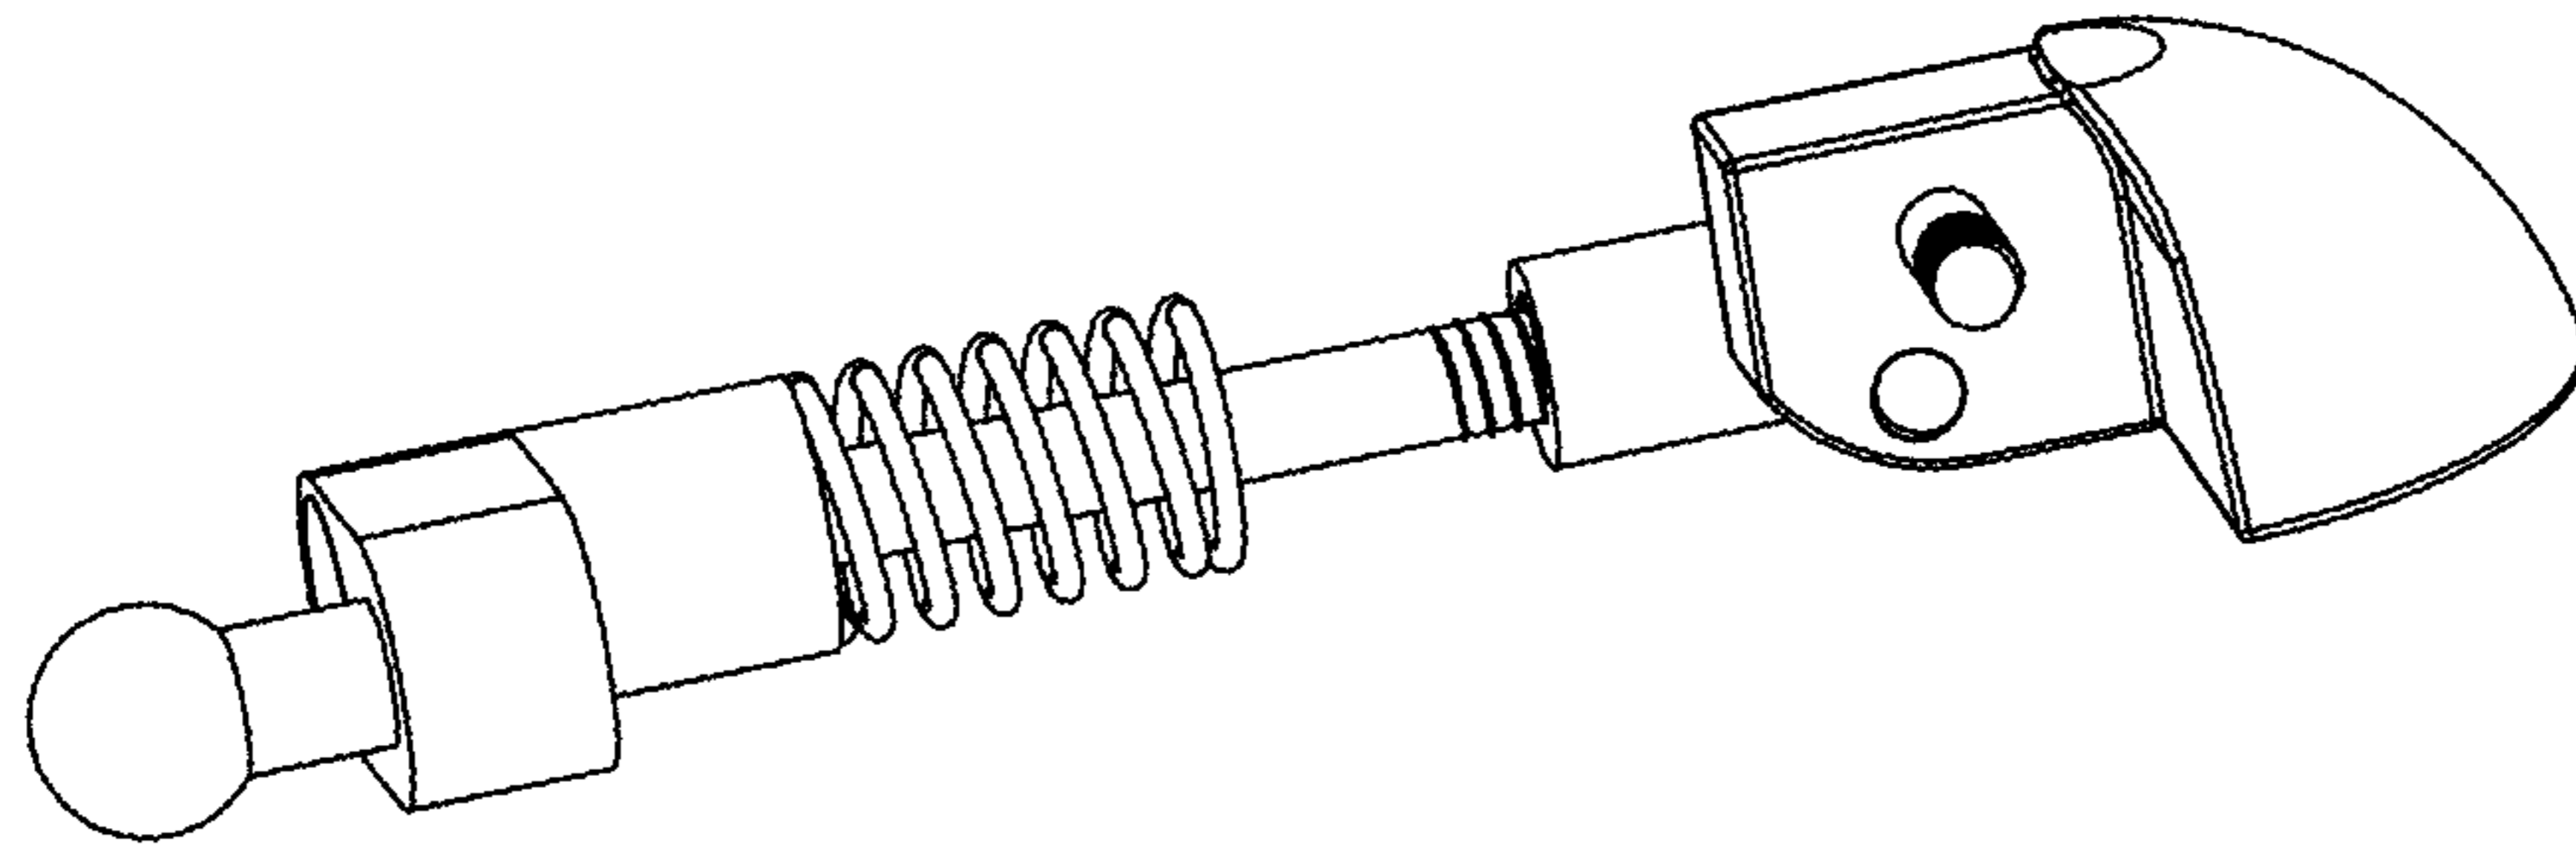


Fig. 46

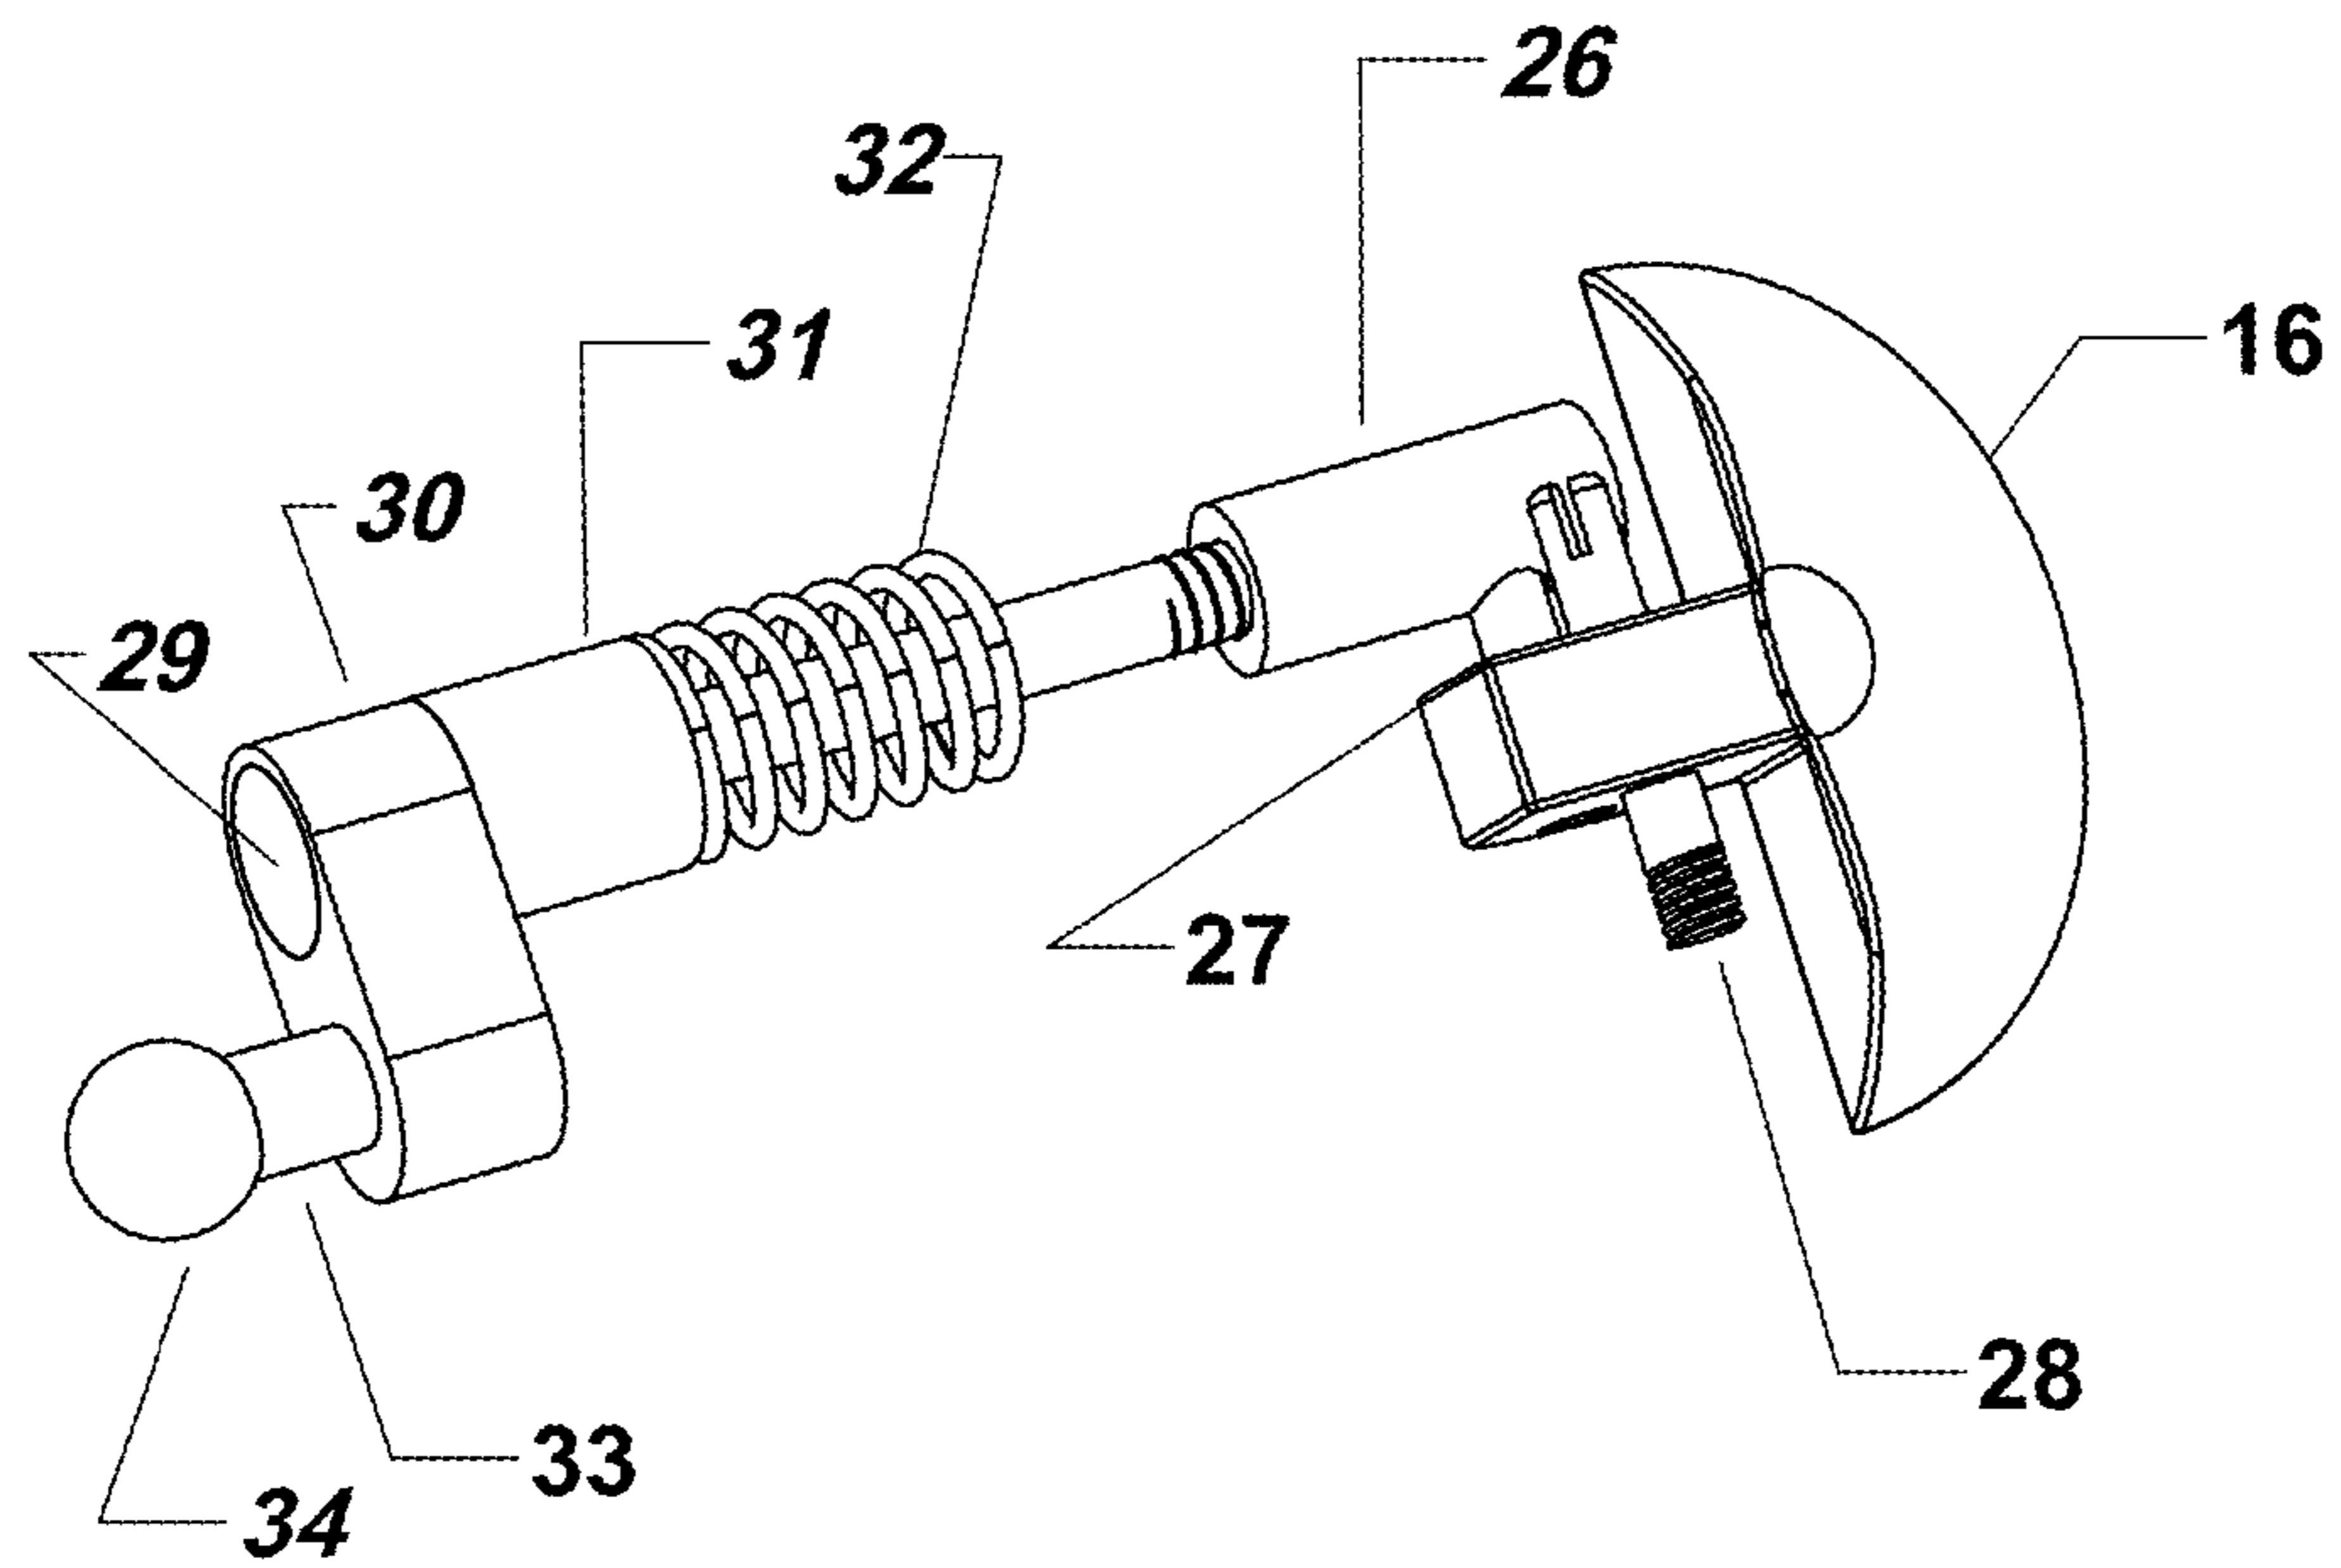


Fig. 47

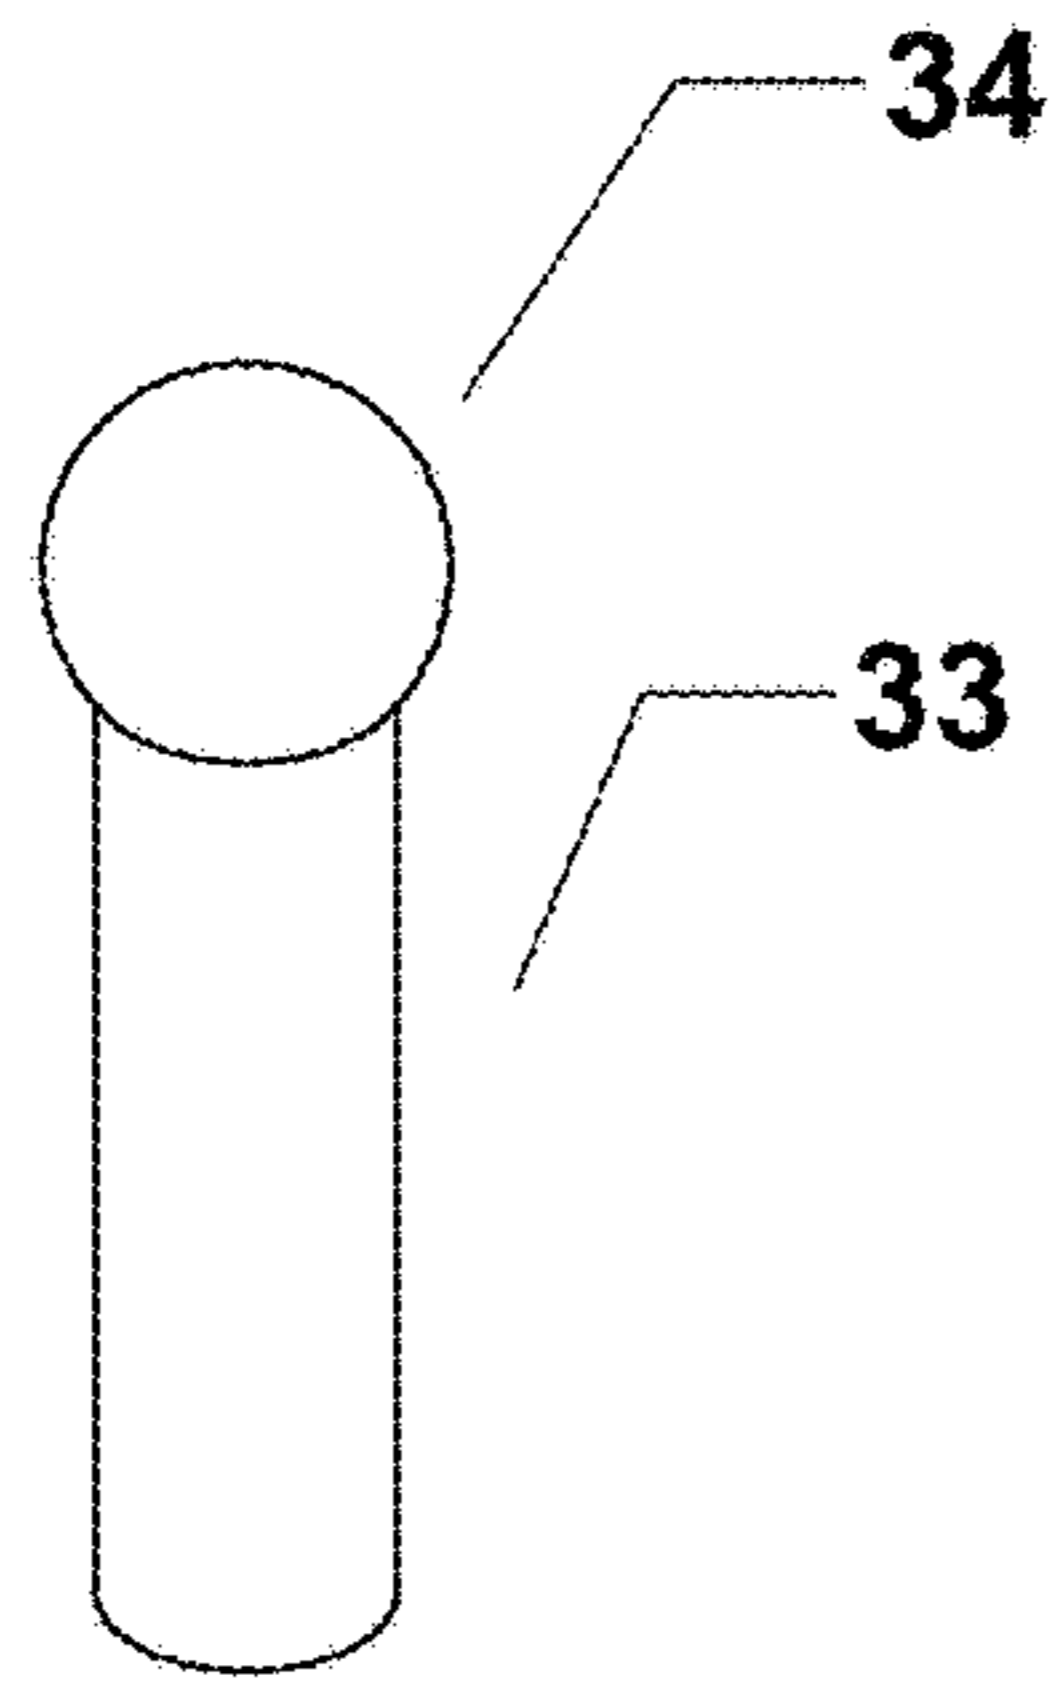


Fig. 48

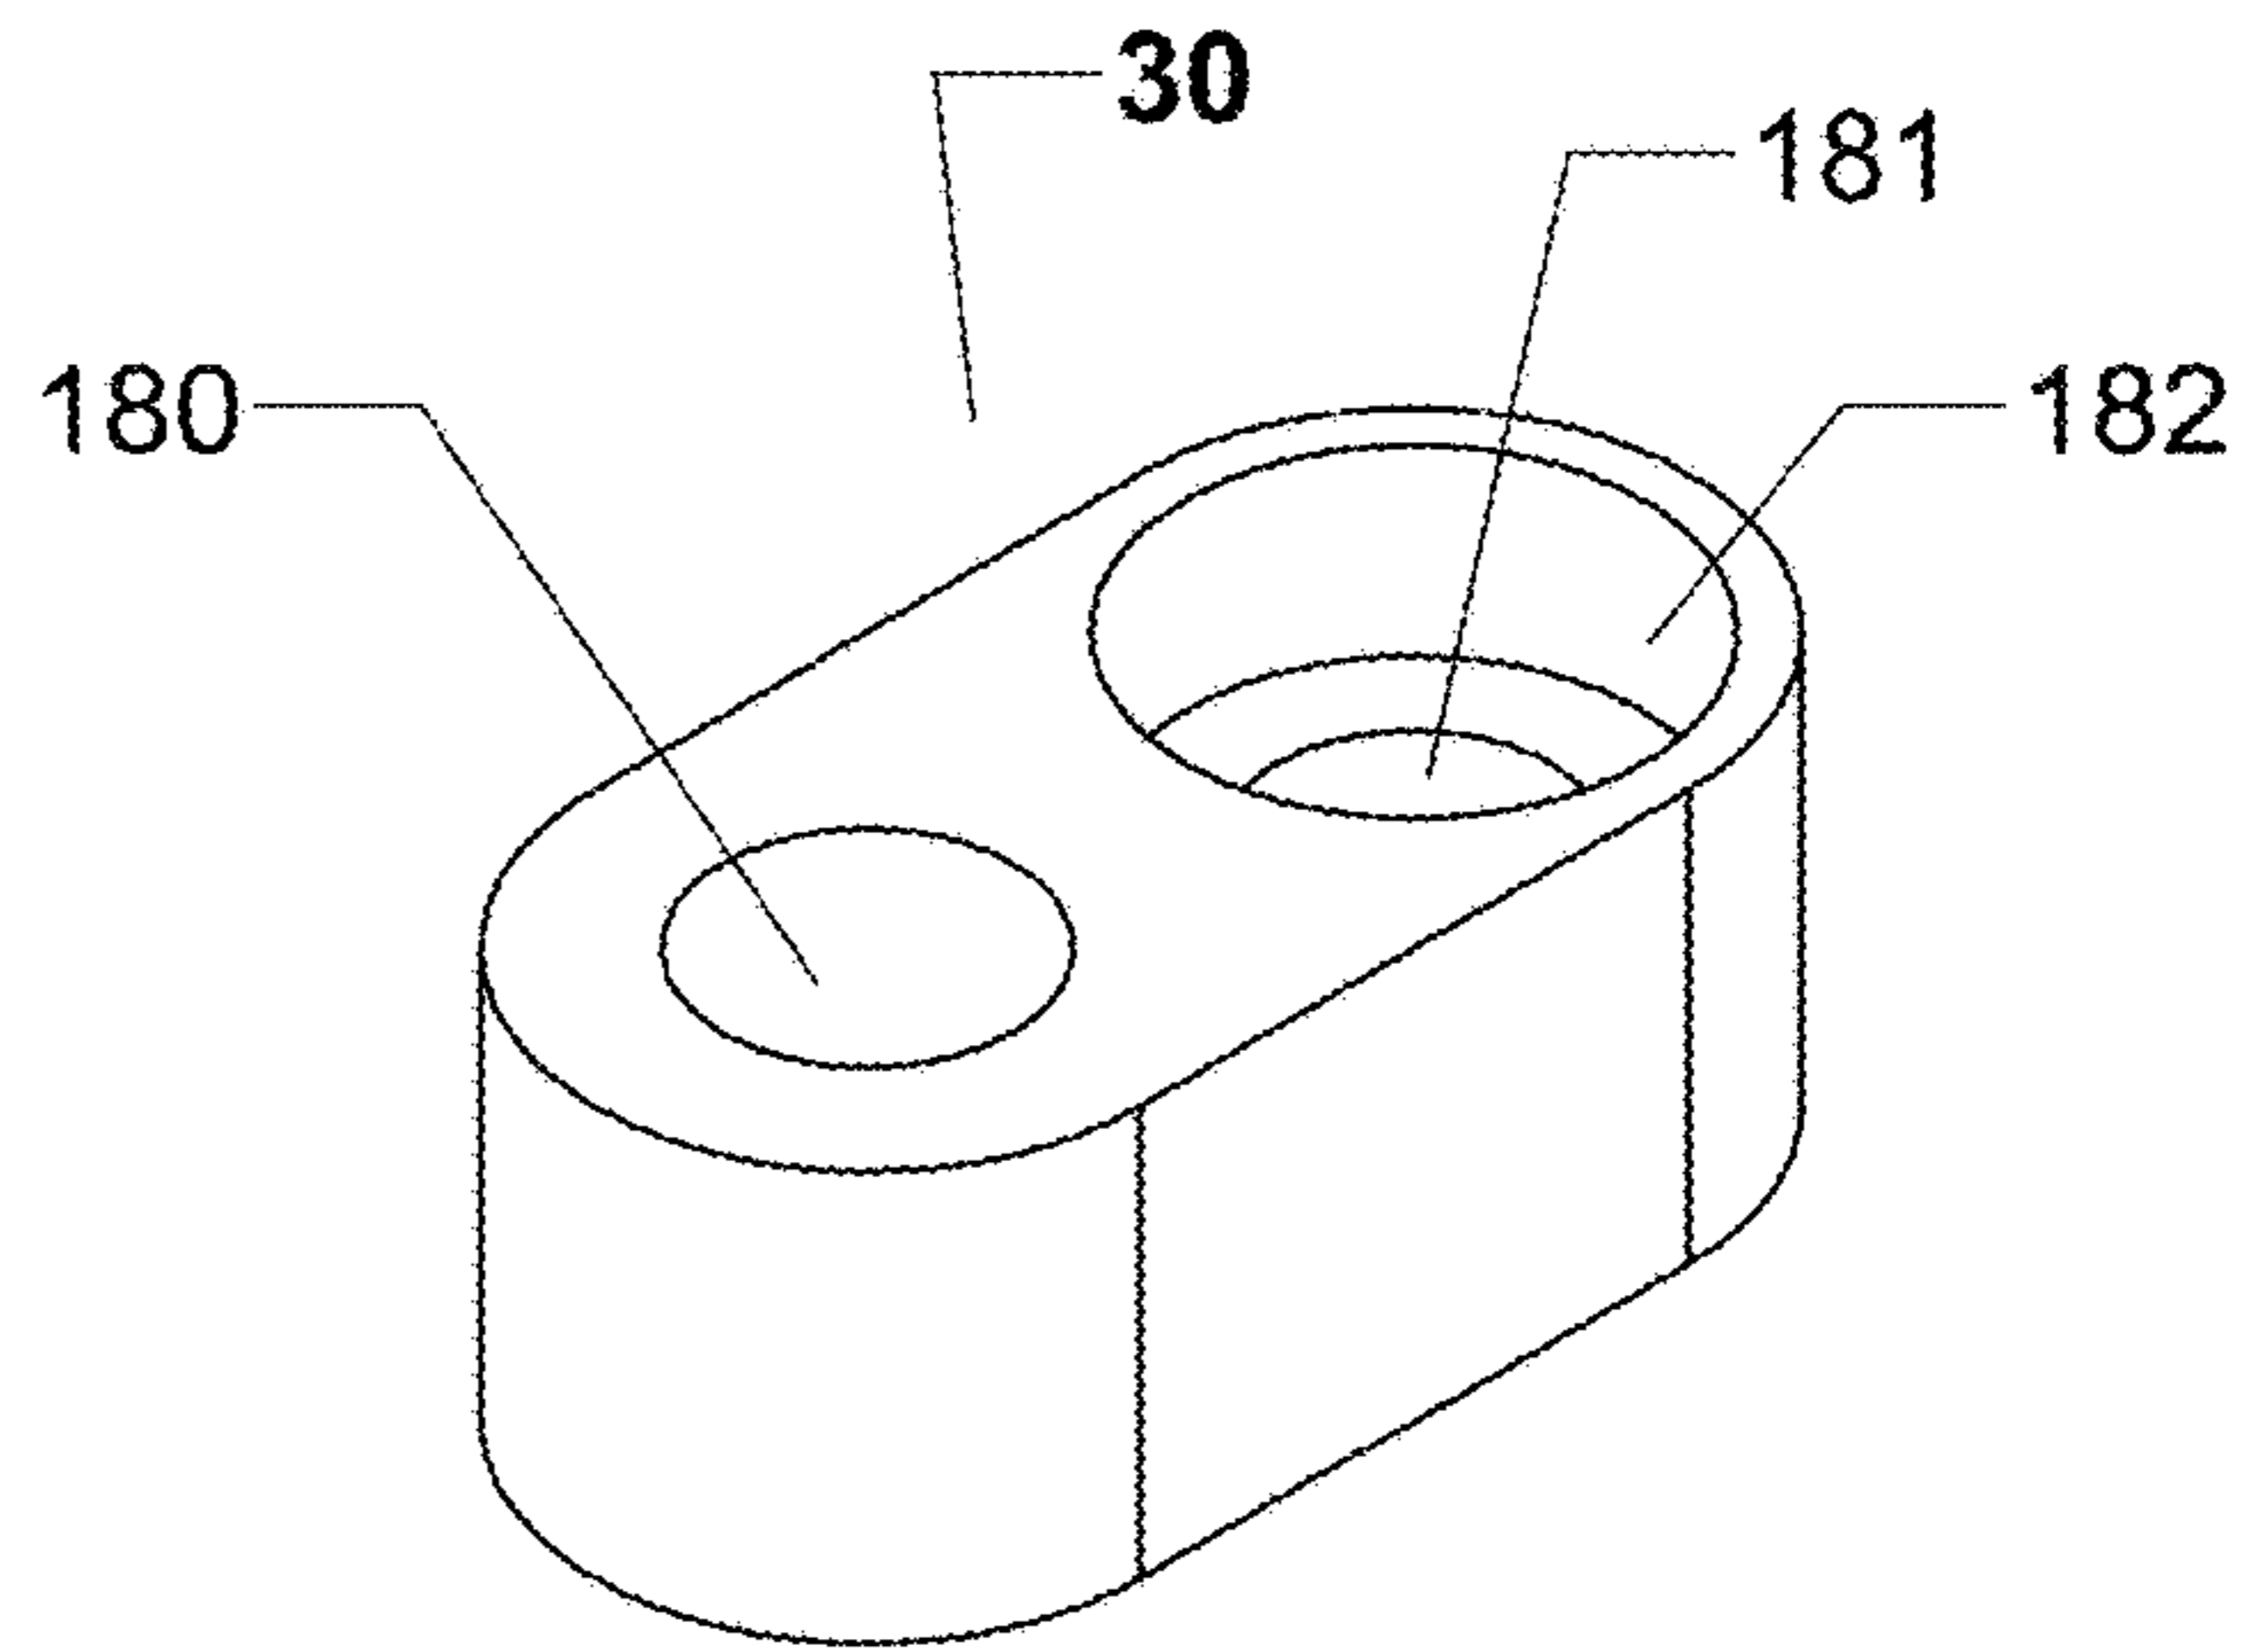


Fig. 49

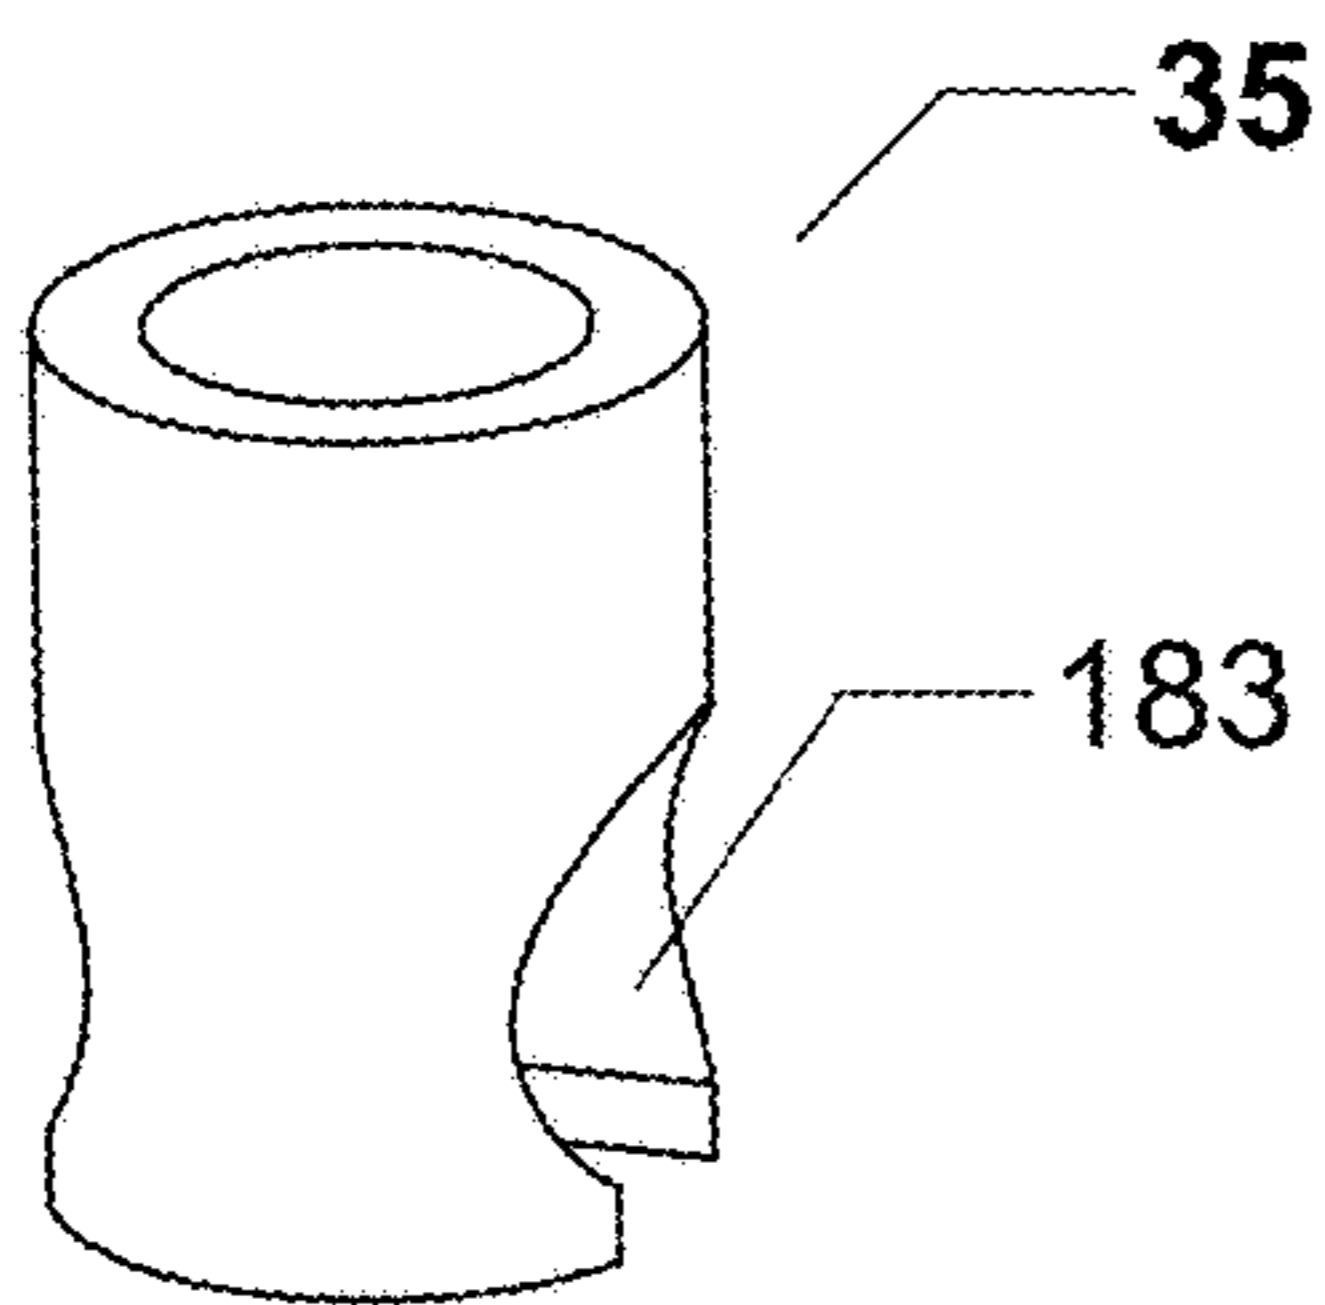


Fig. 50

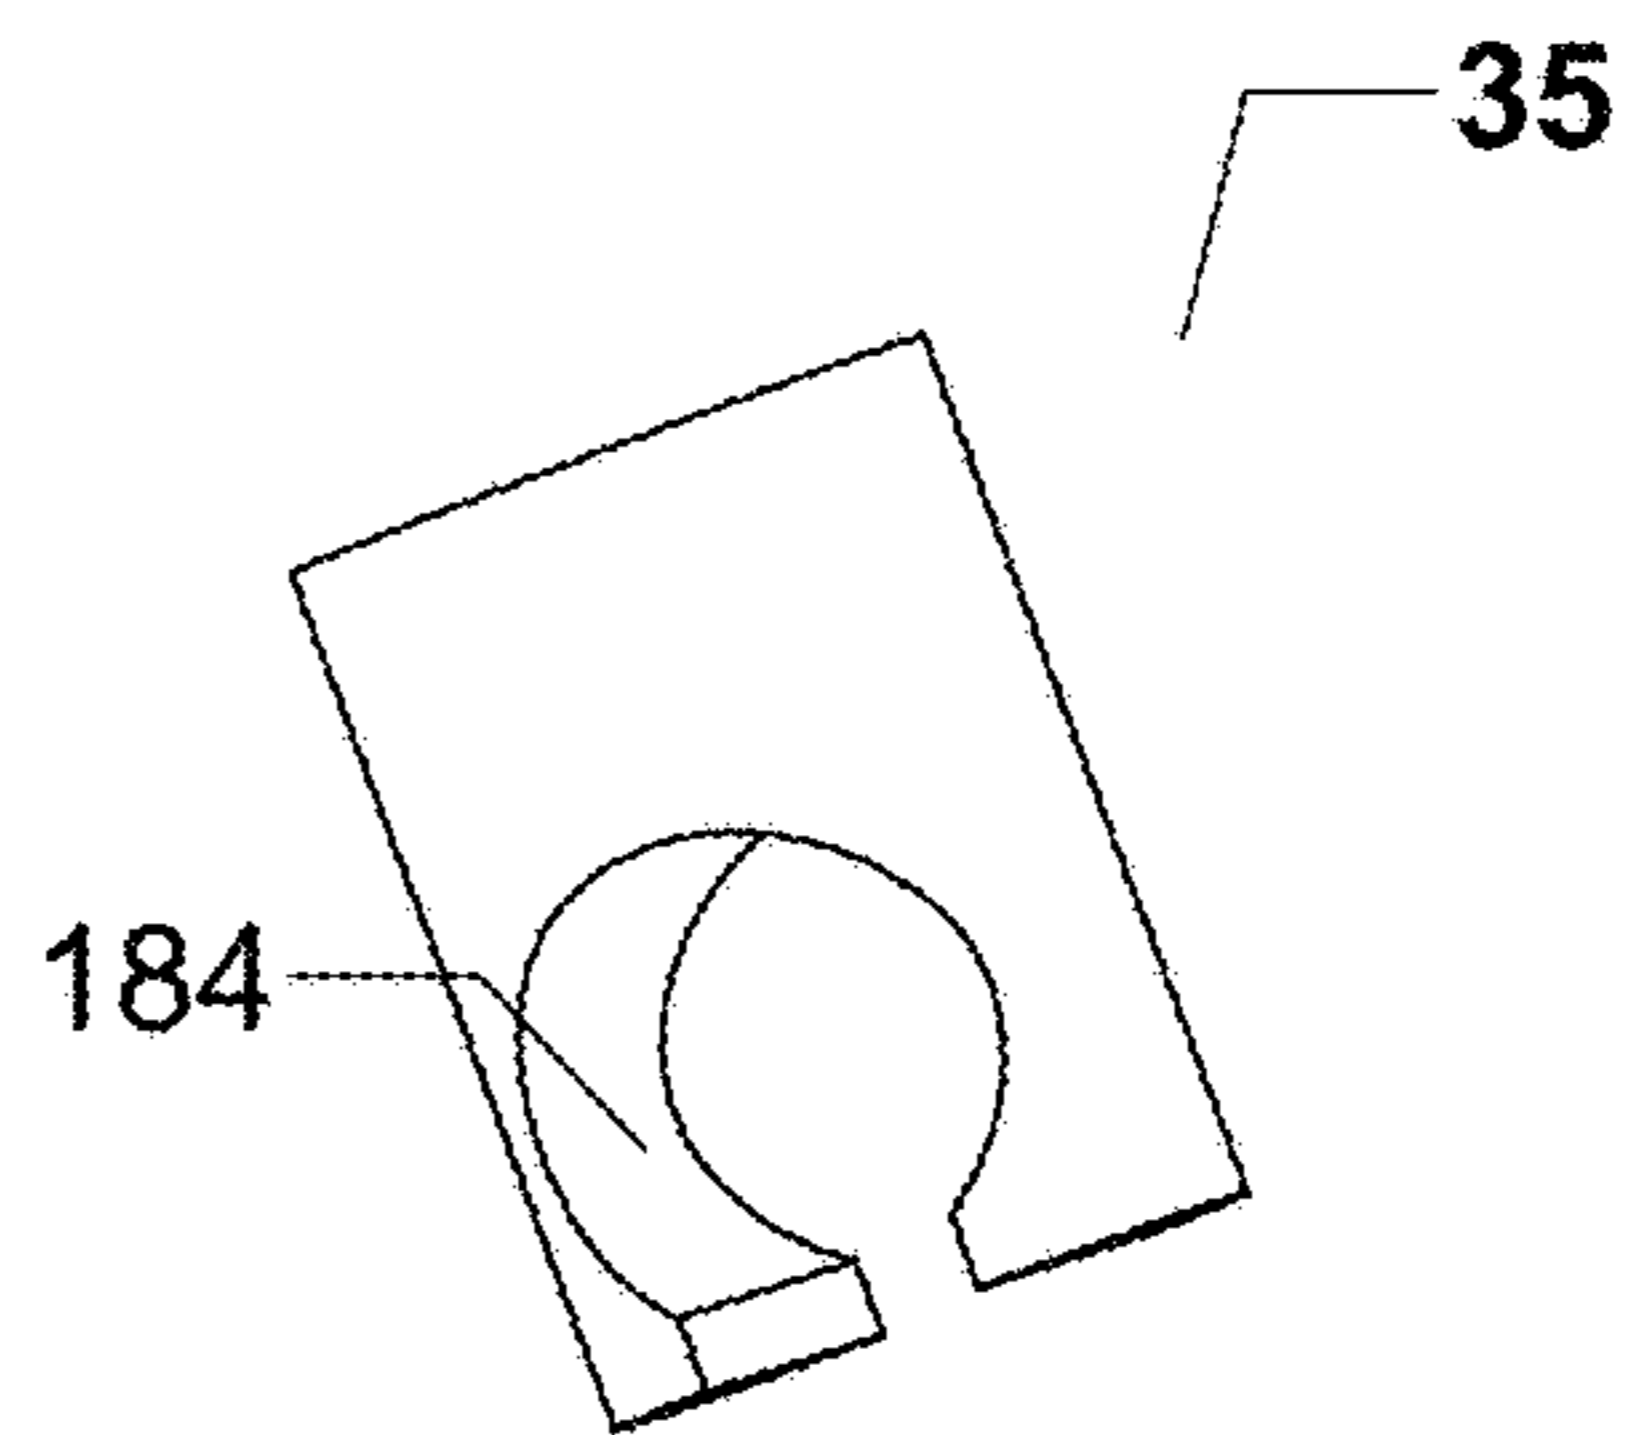


Fig. 51

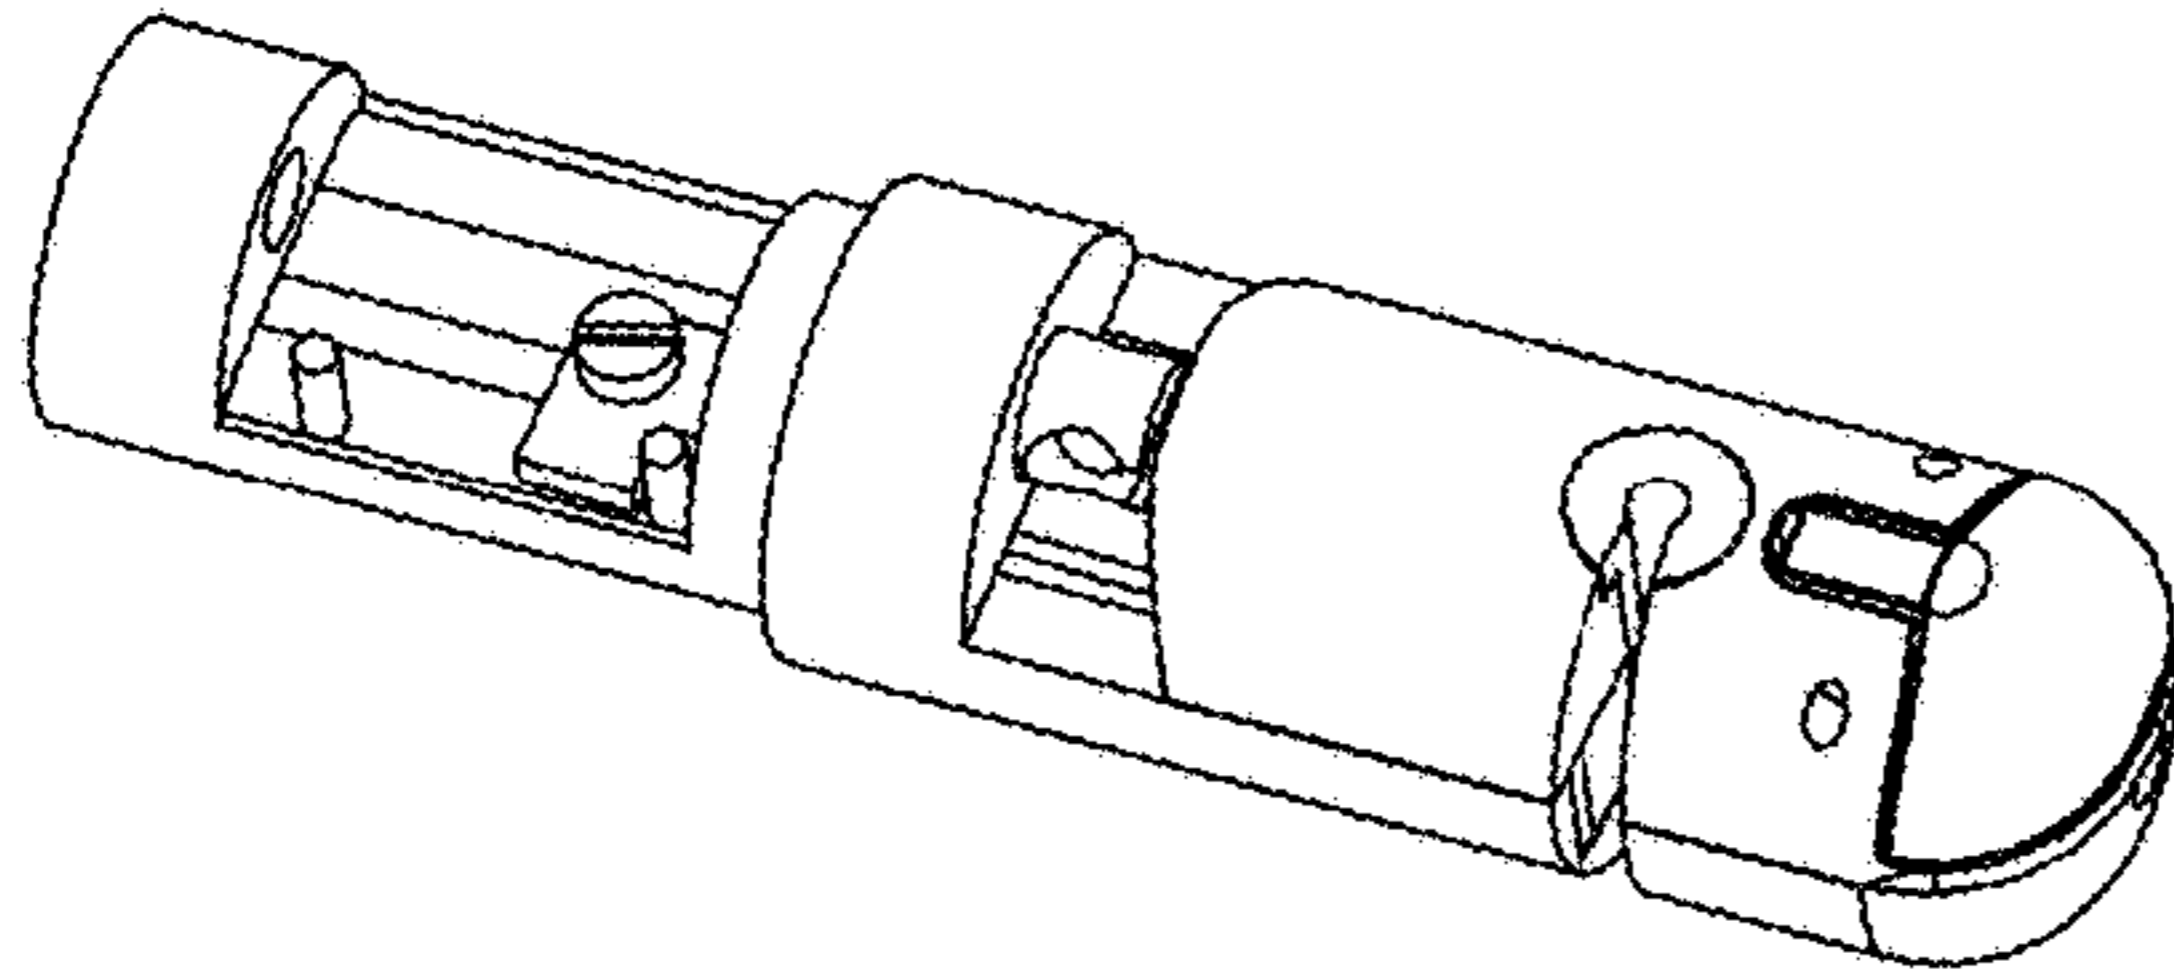


Fig. 52

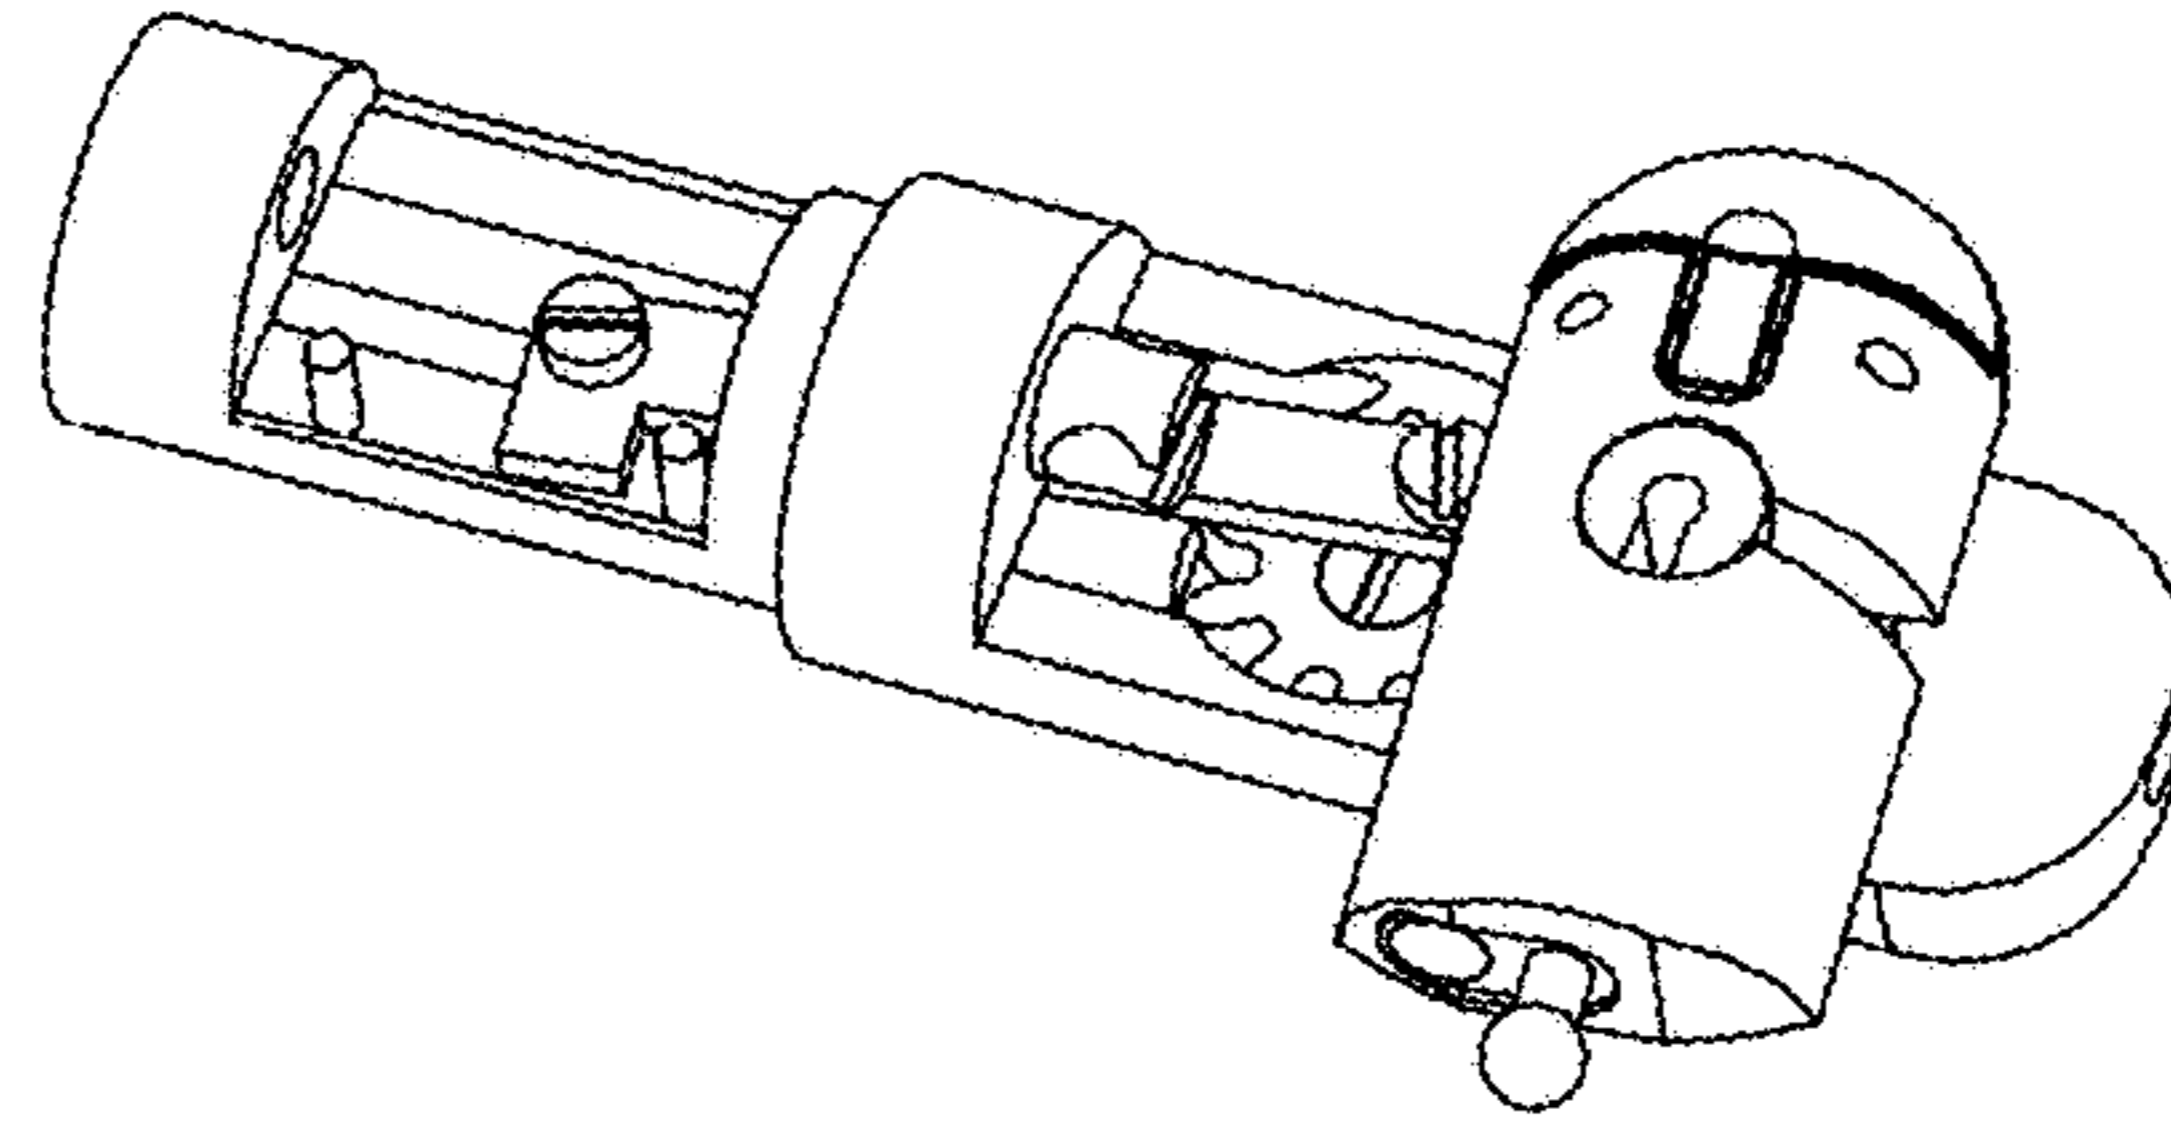


Fig. 53

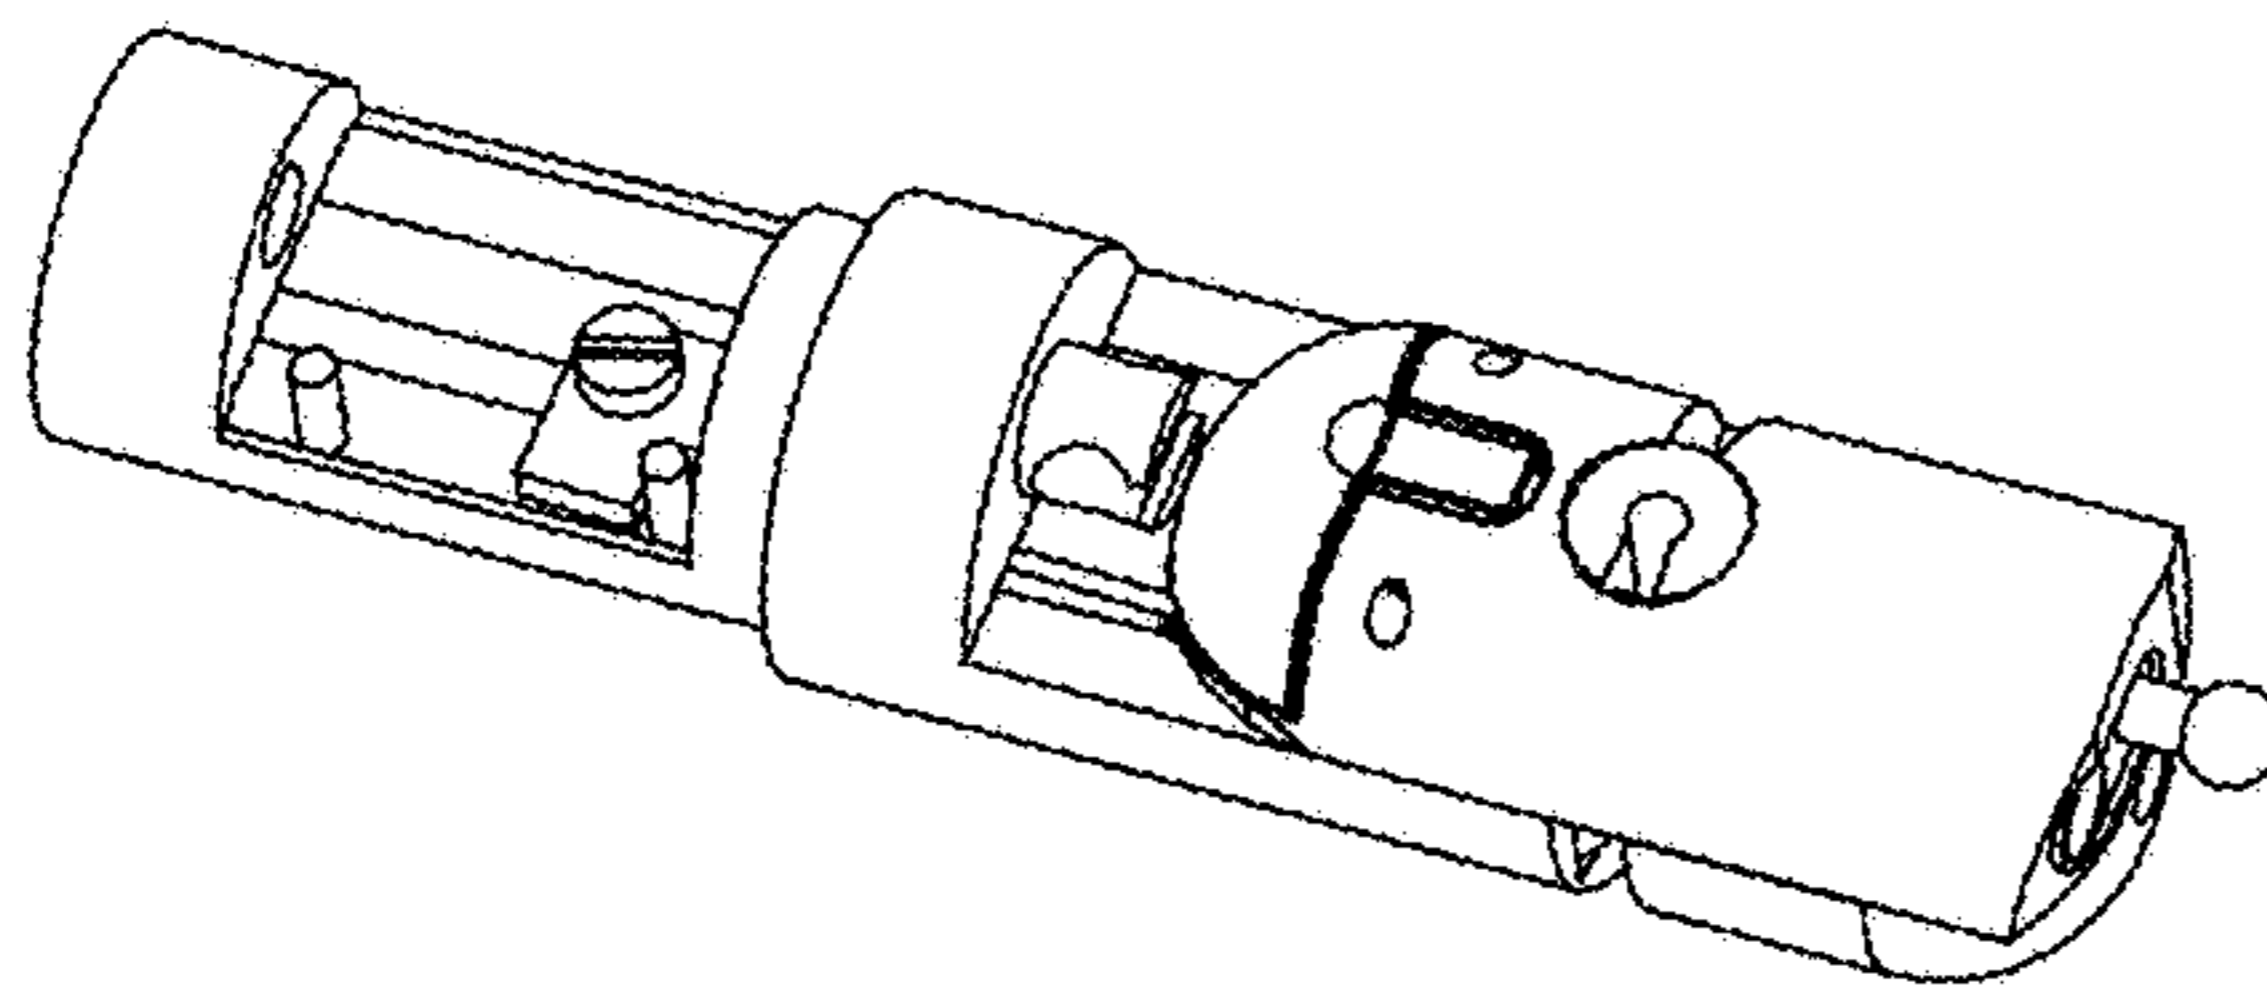


Fig. 54

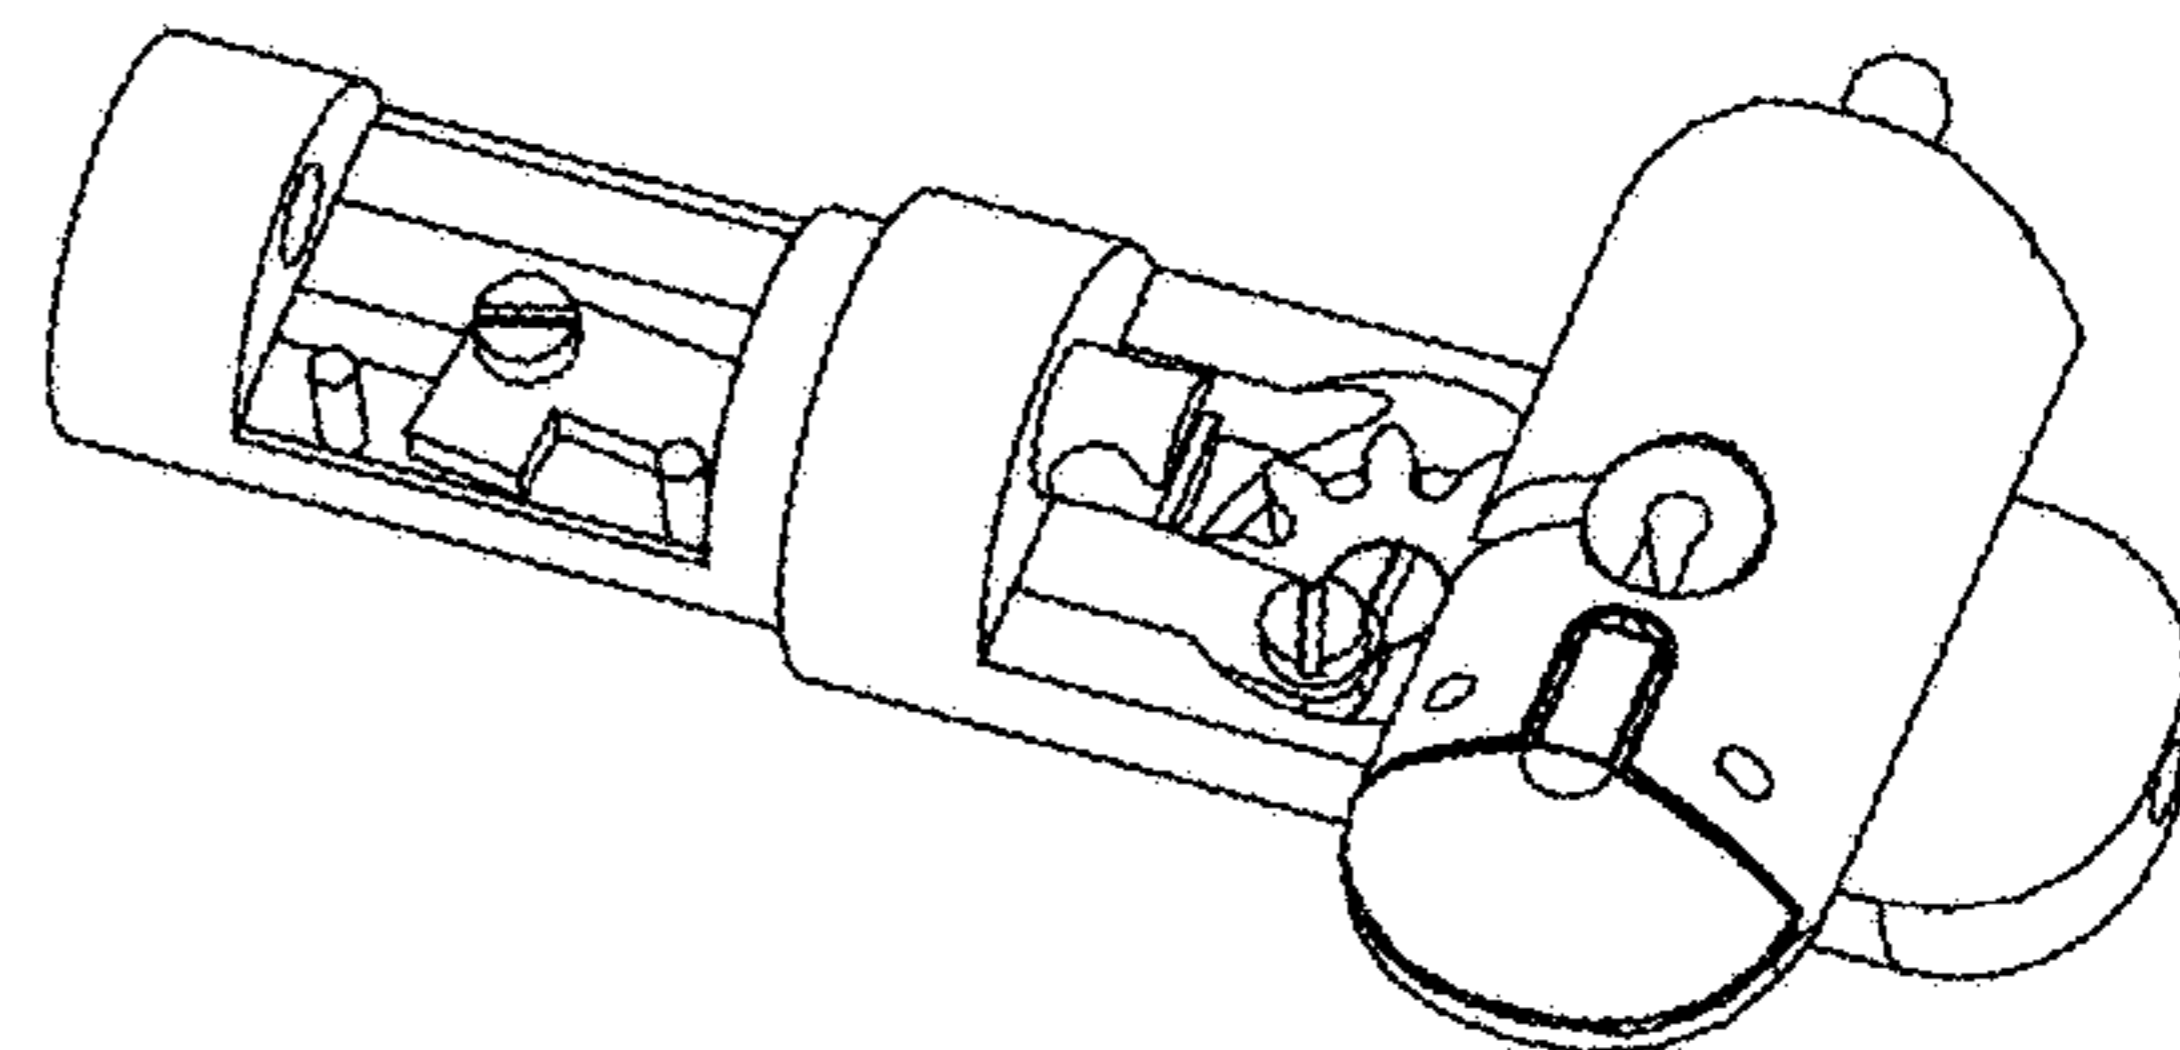


Fig. 55

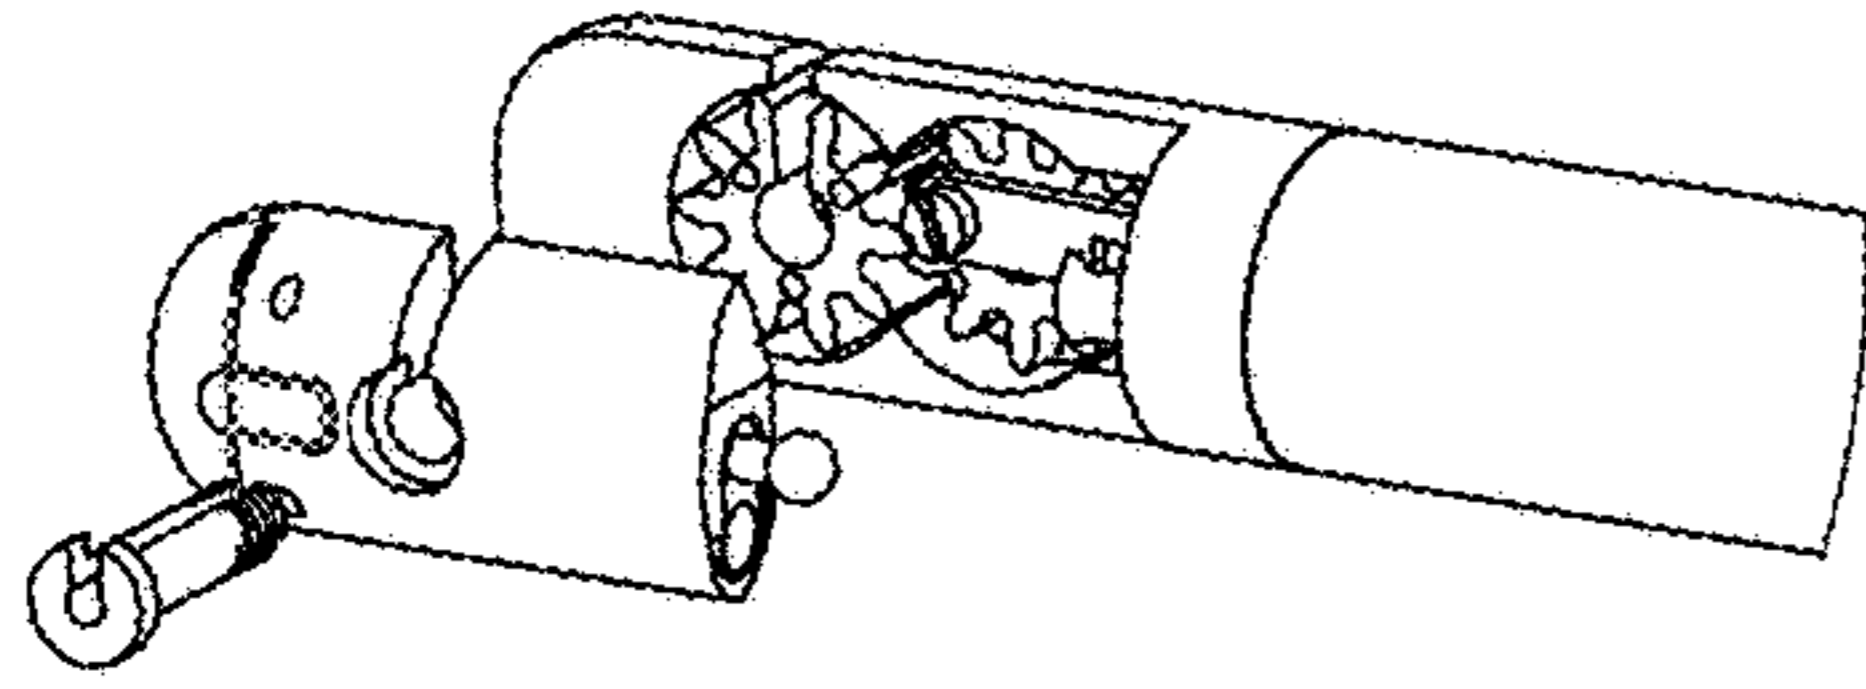


Fig. 56

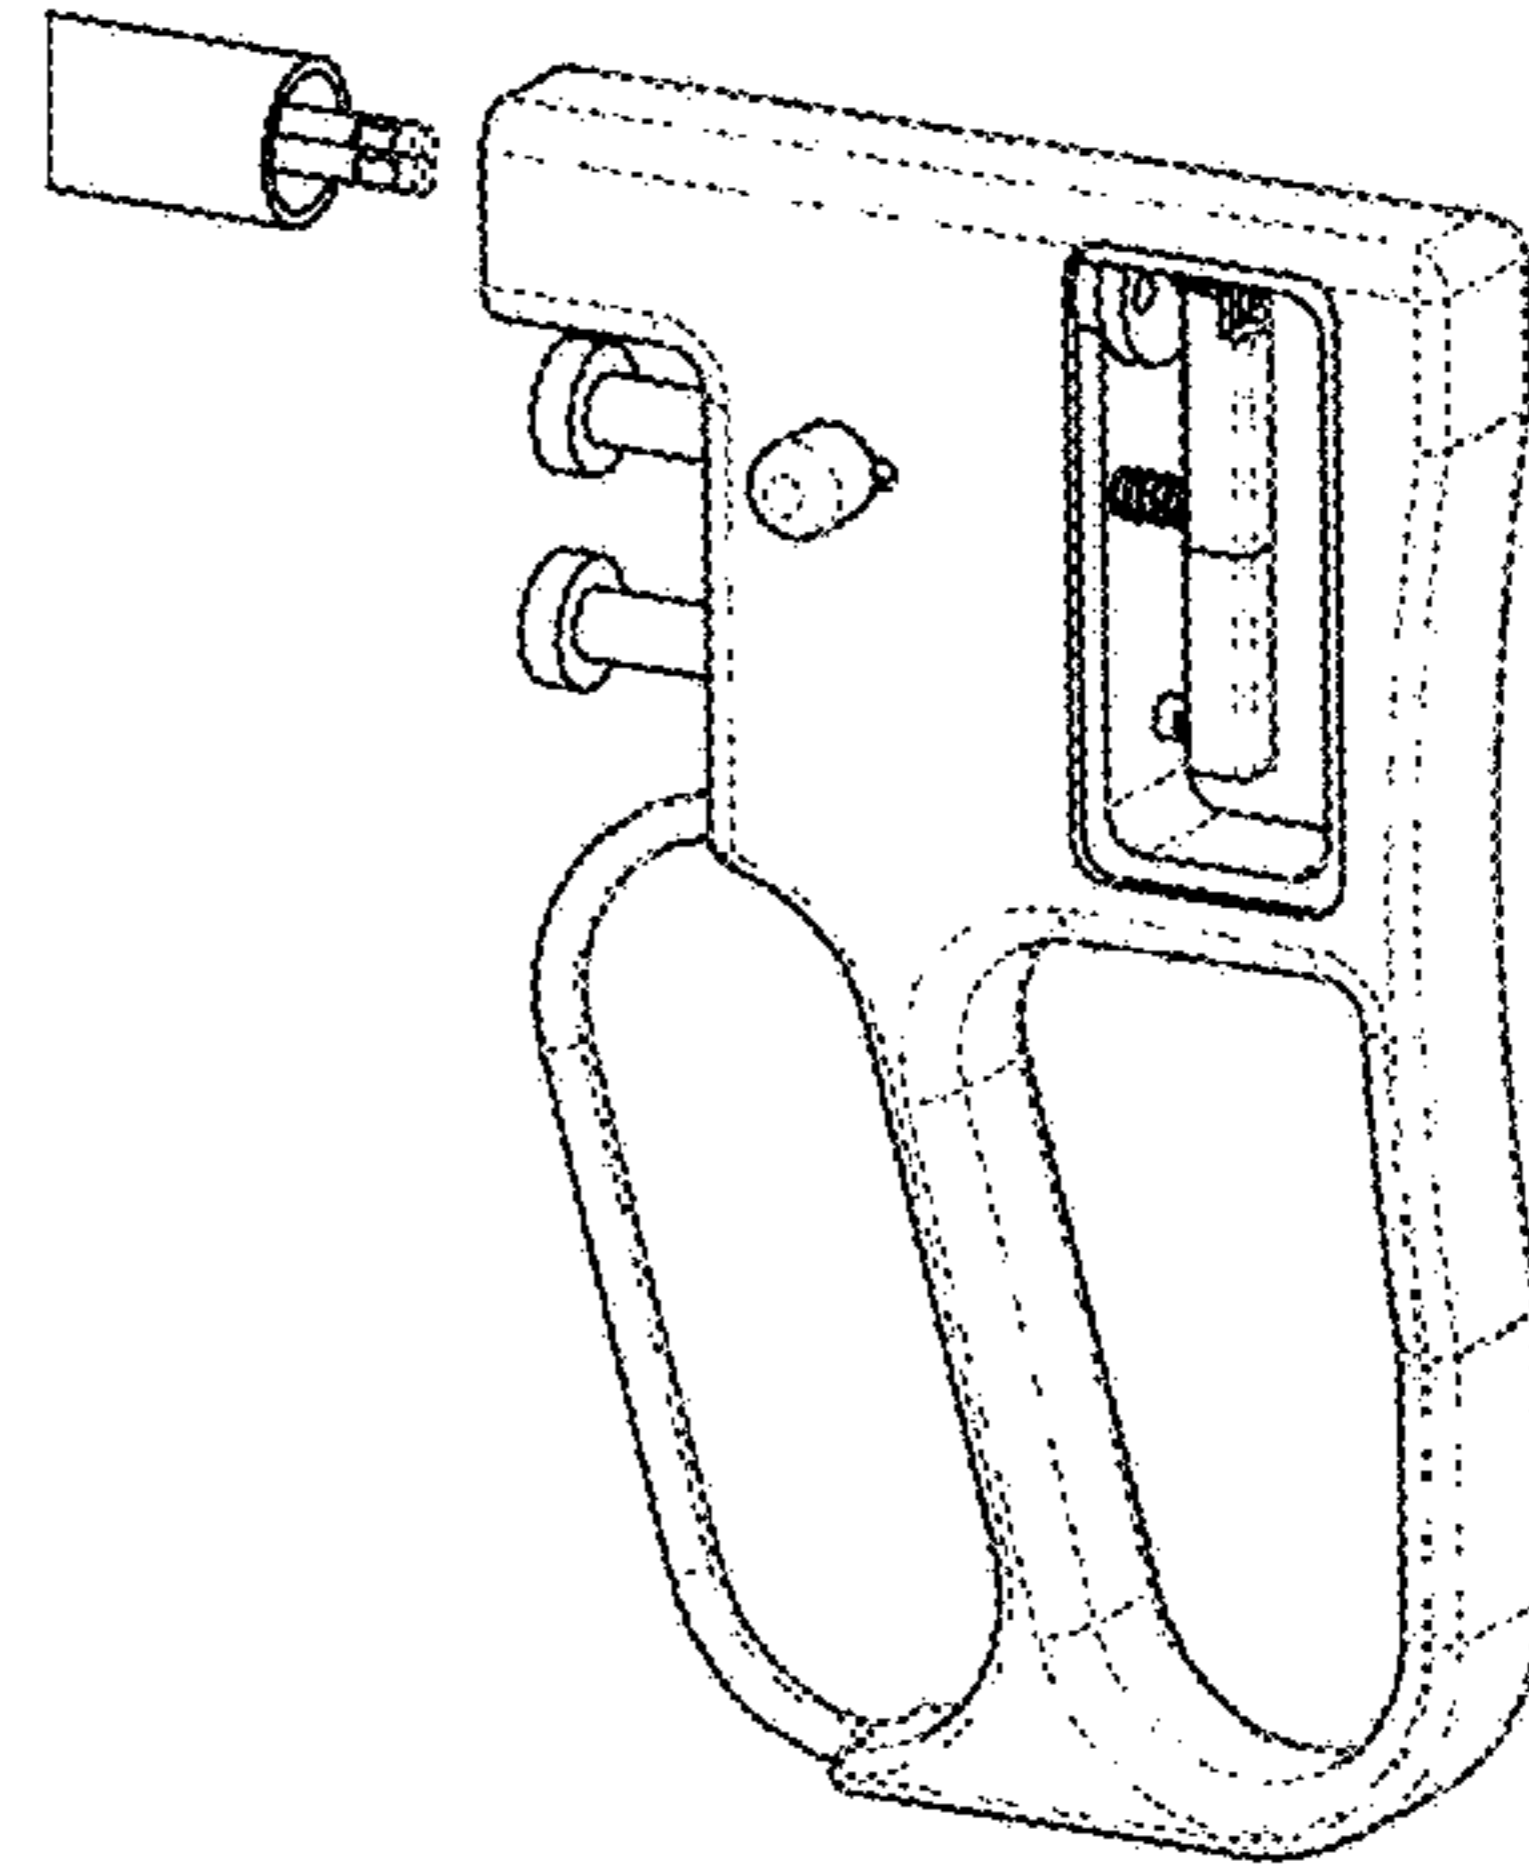


Fig. 57

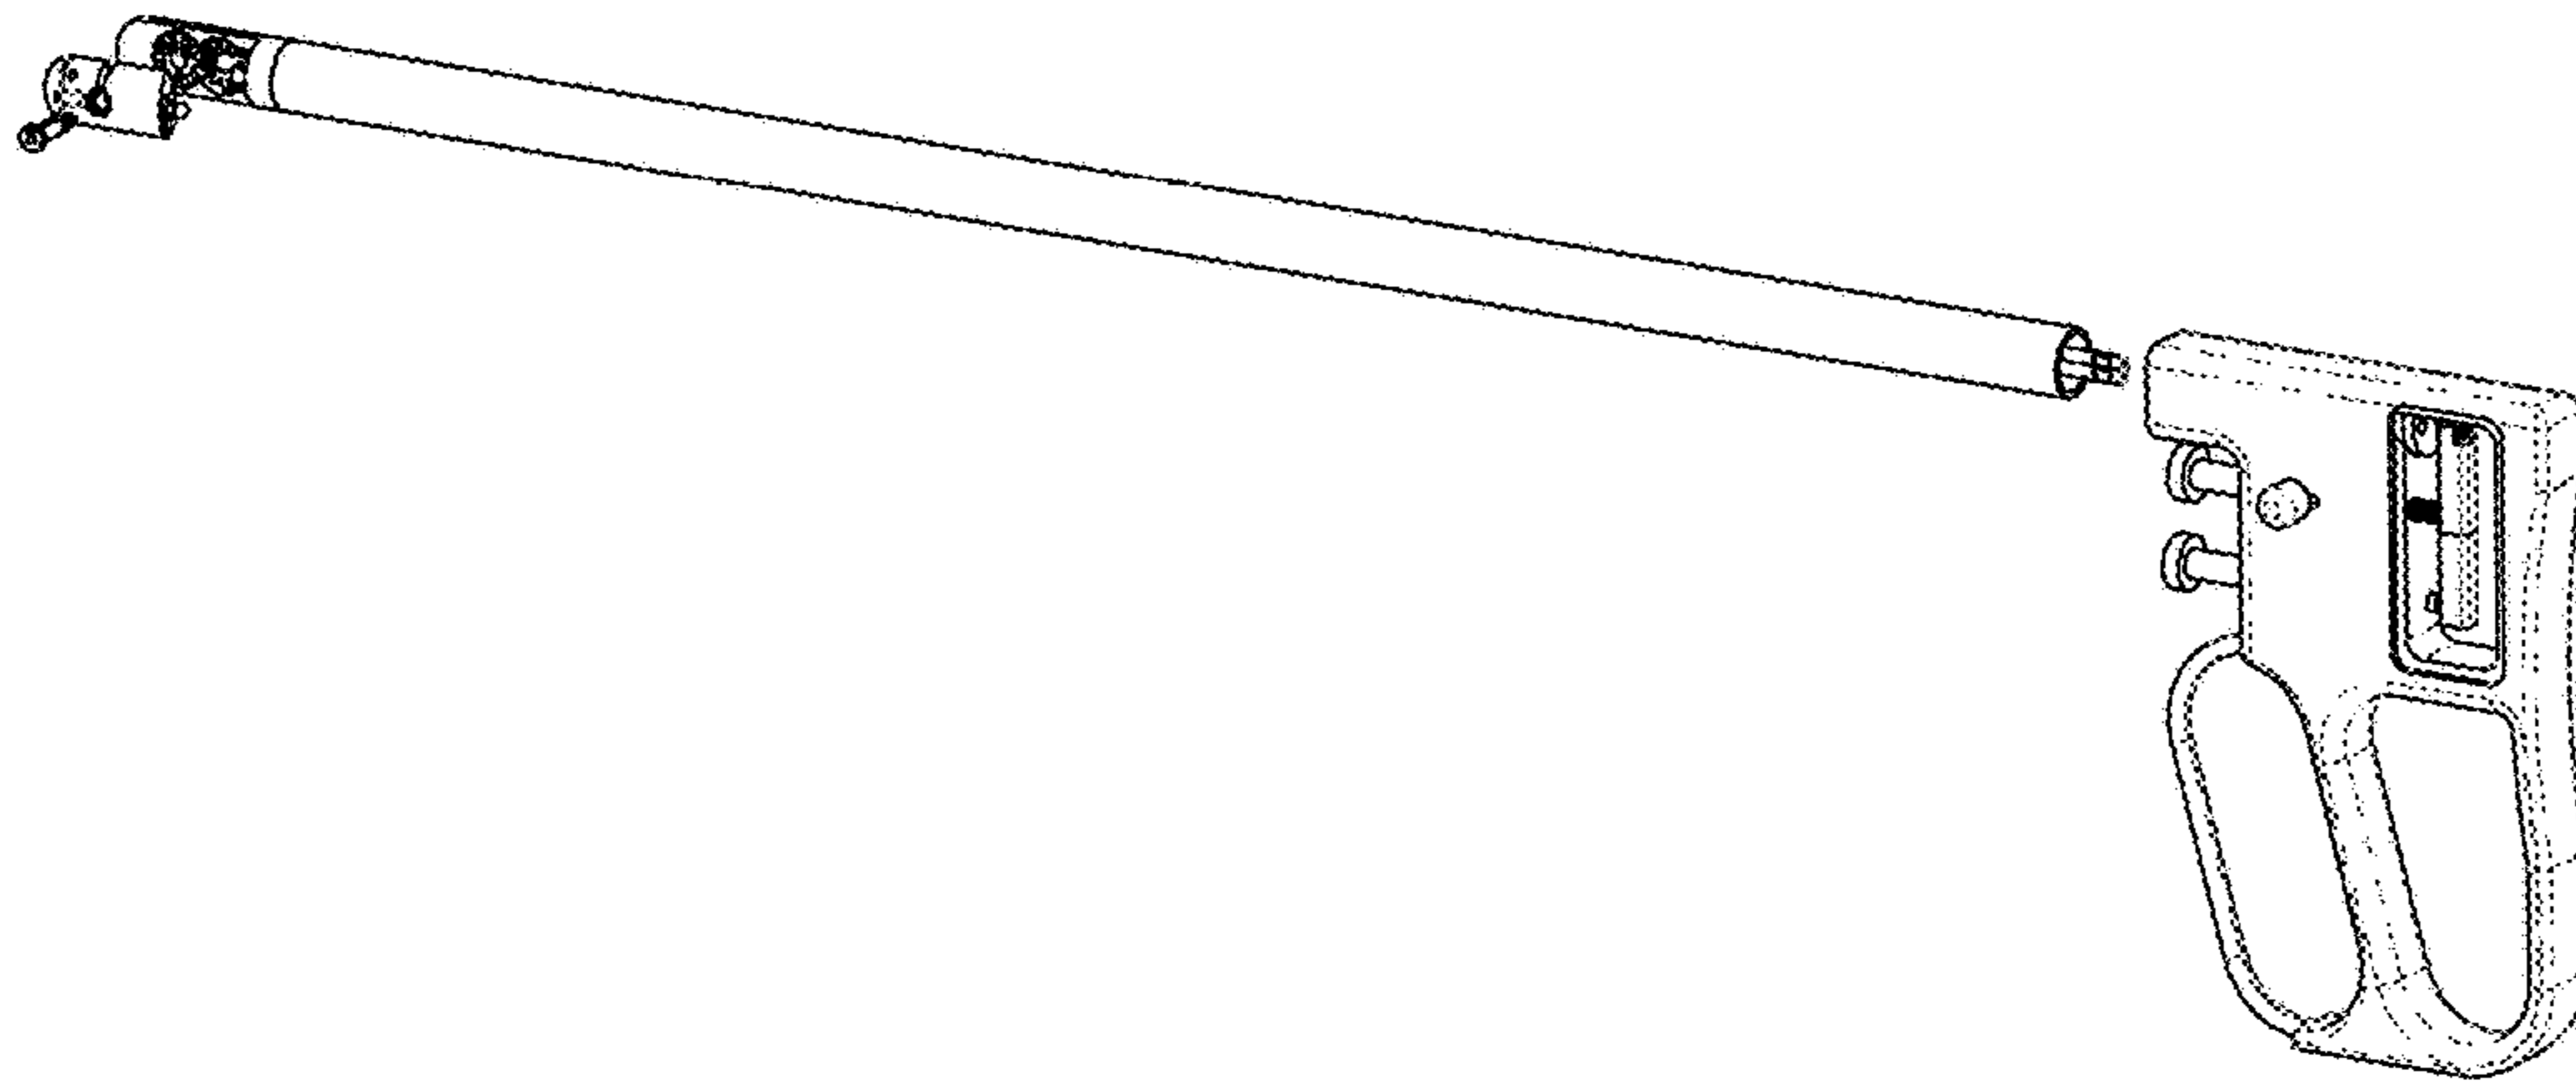


Fig. 58

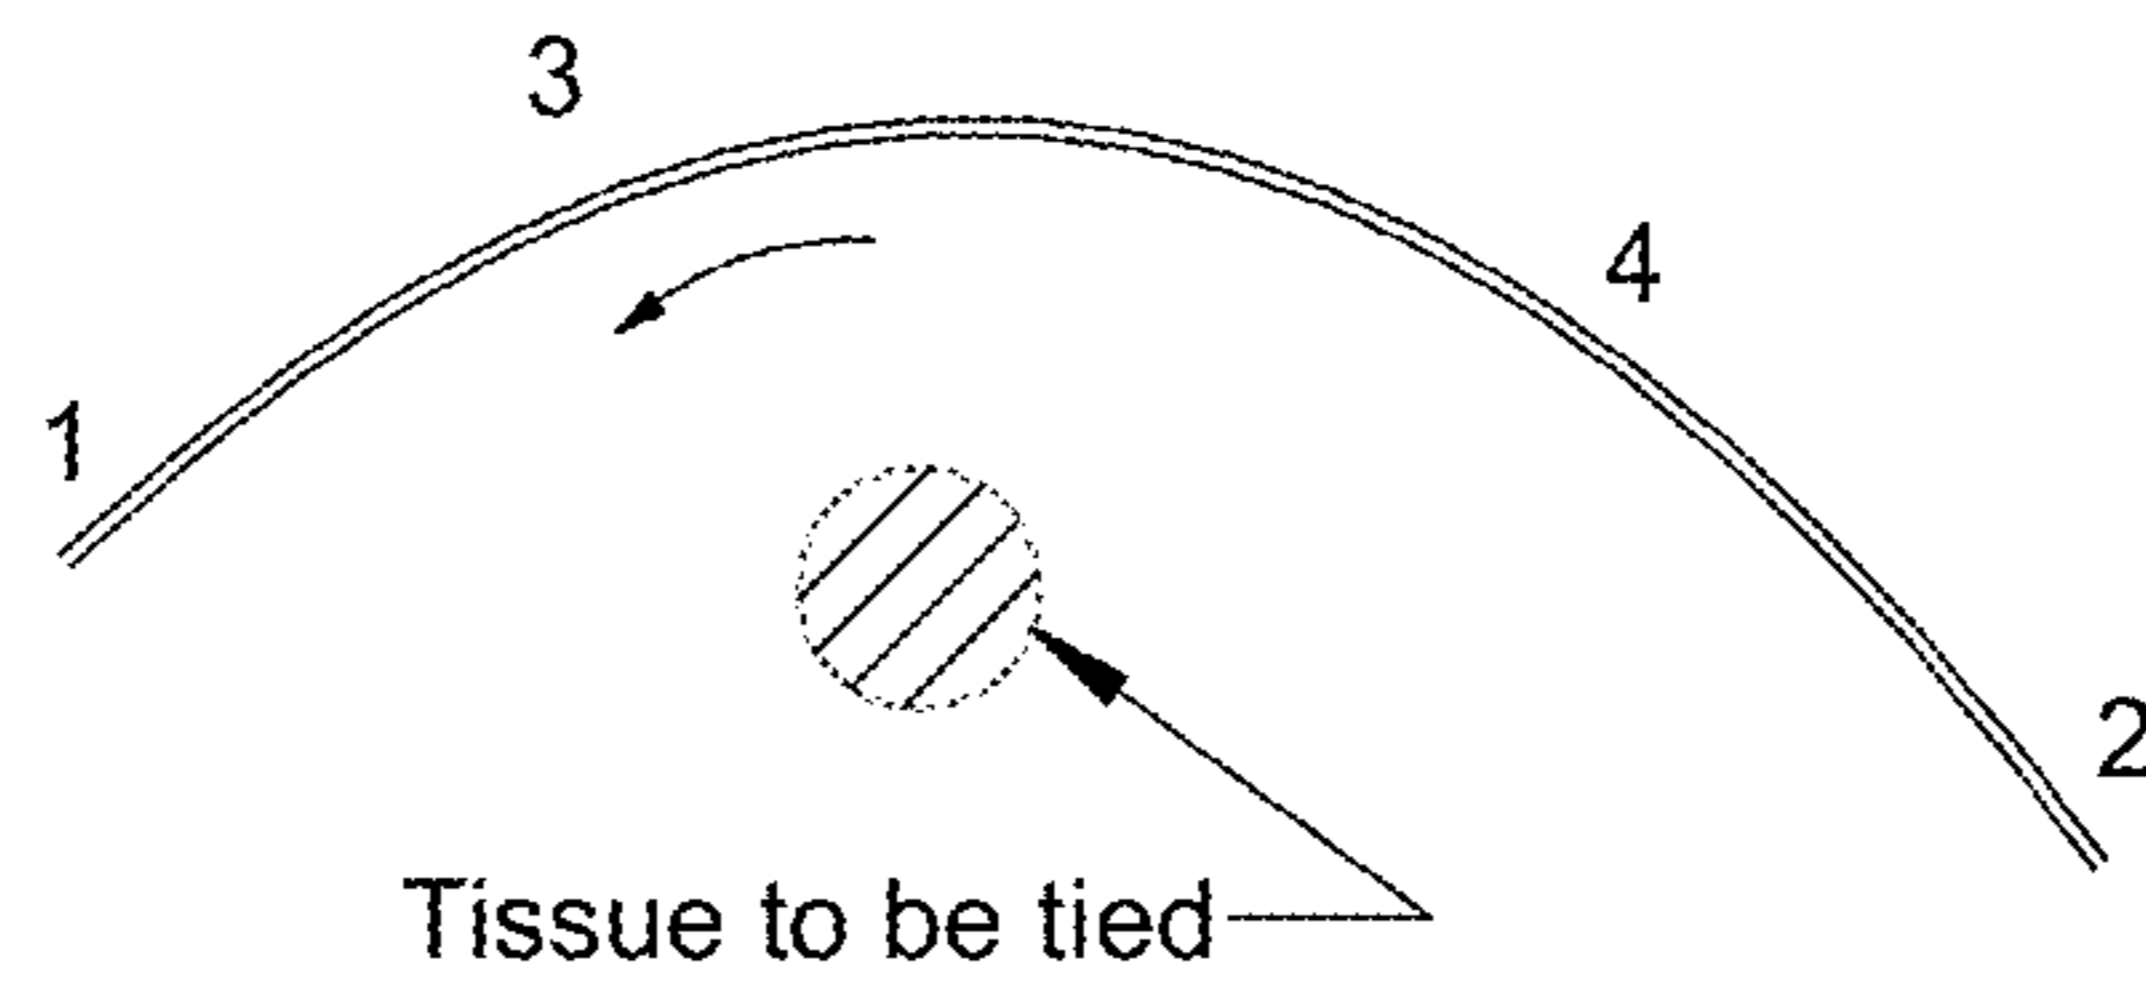


Fig. 59

PRIOR ART

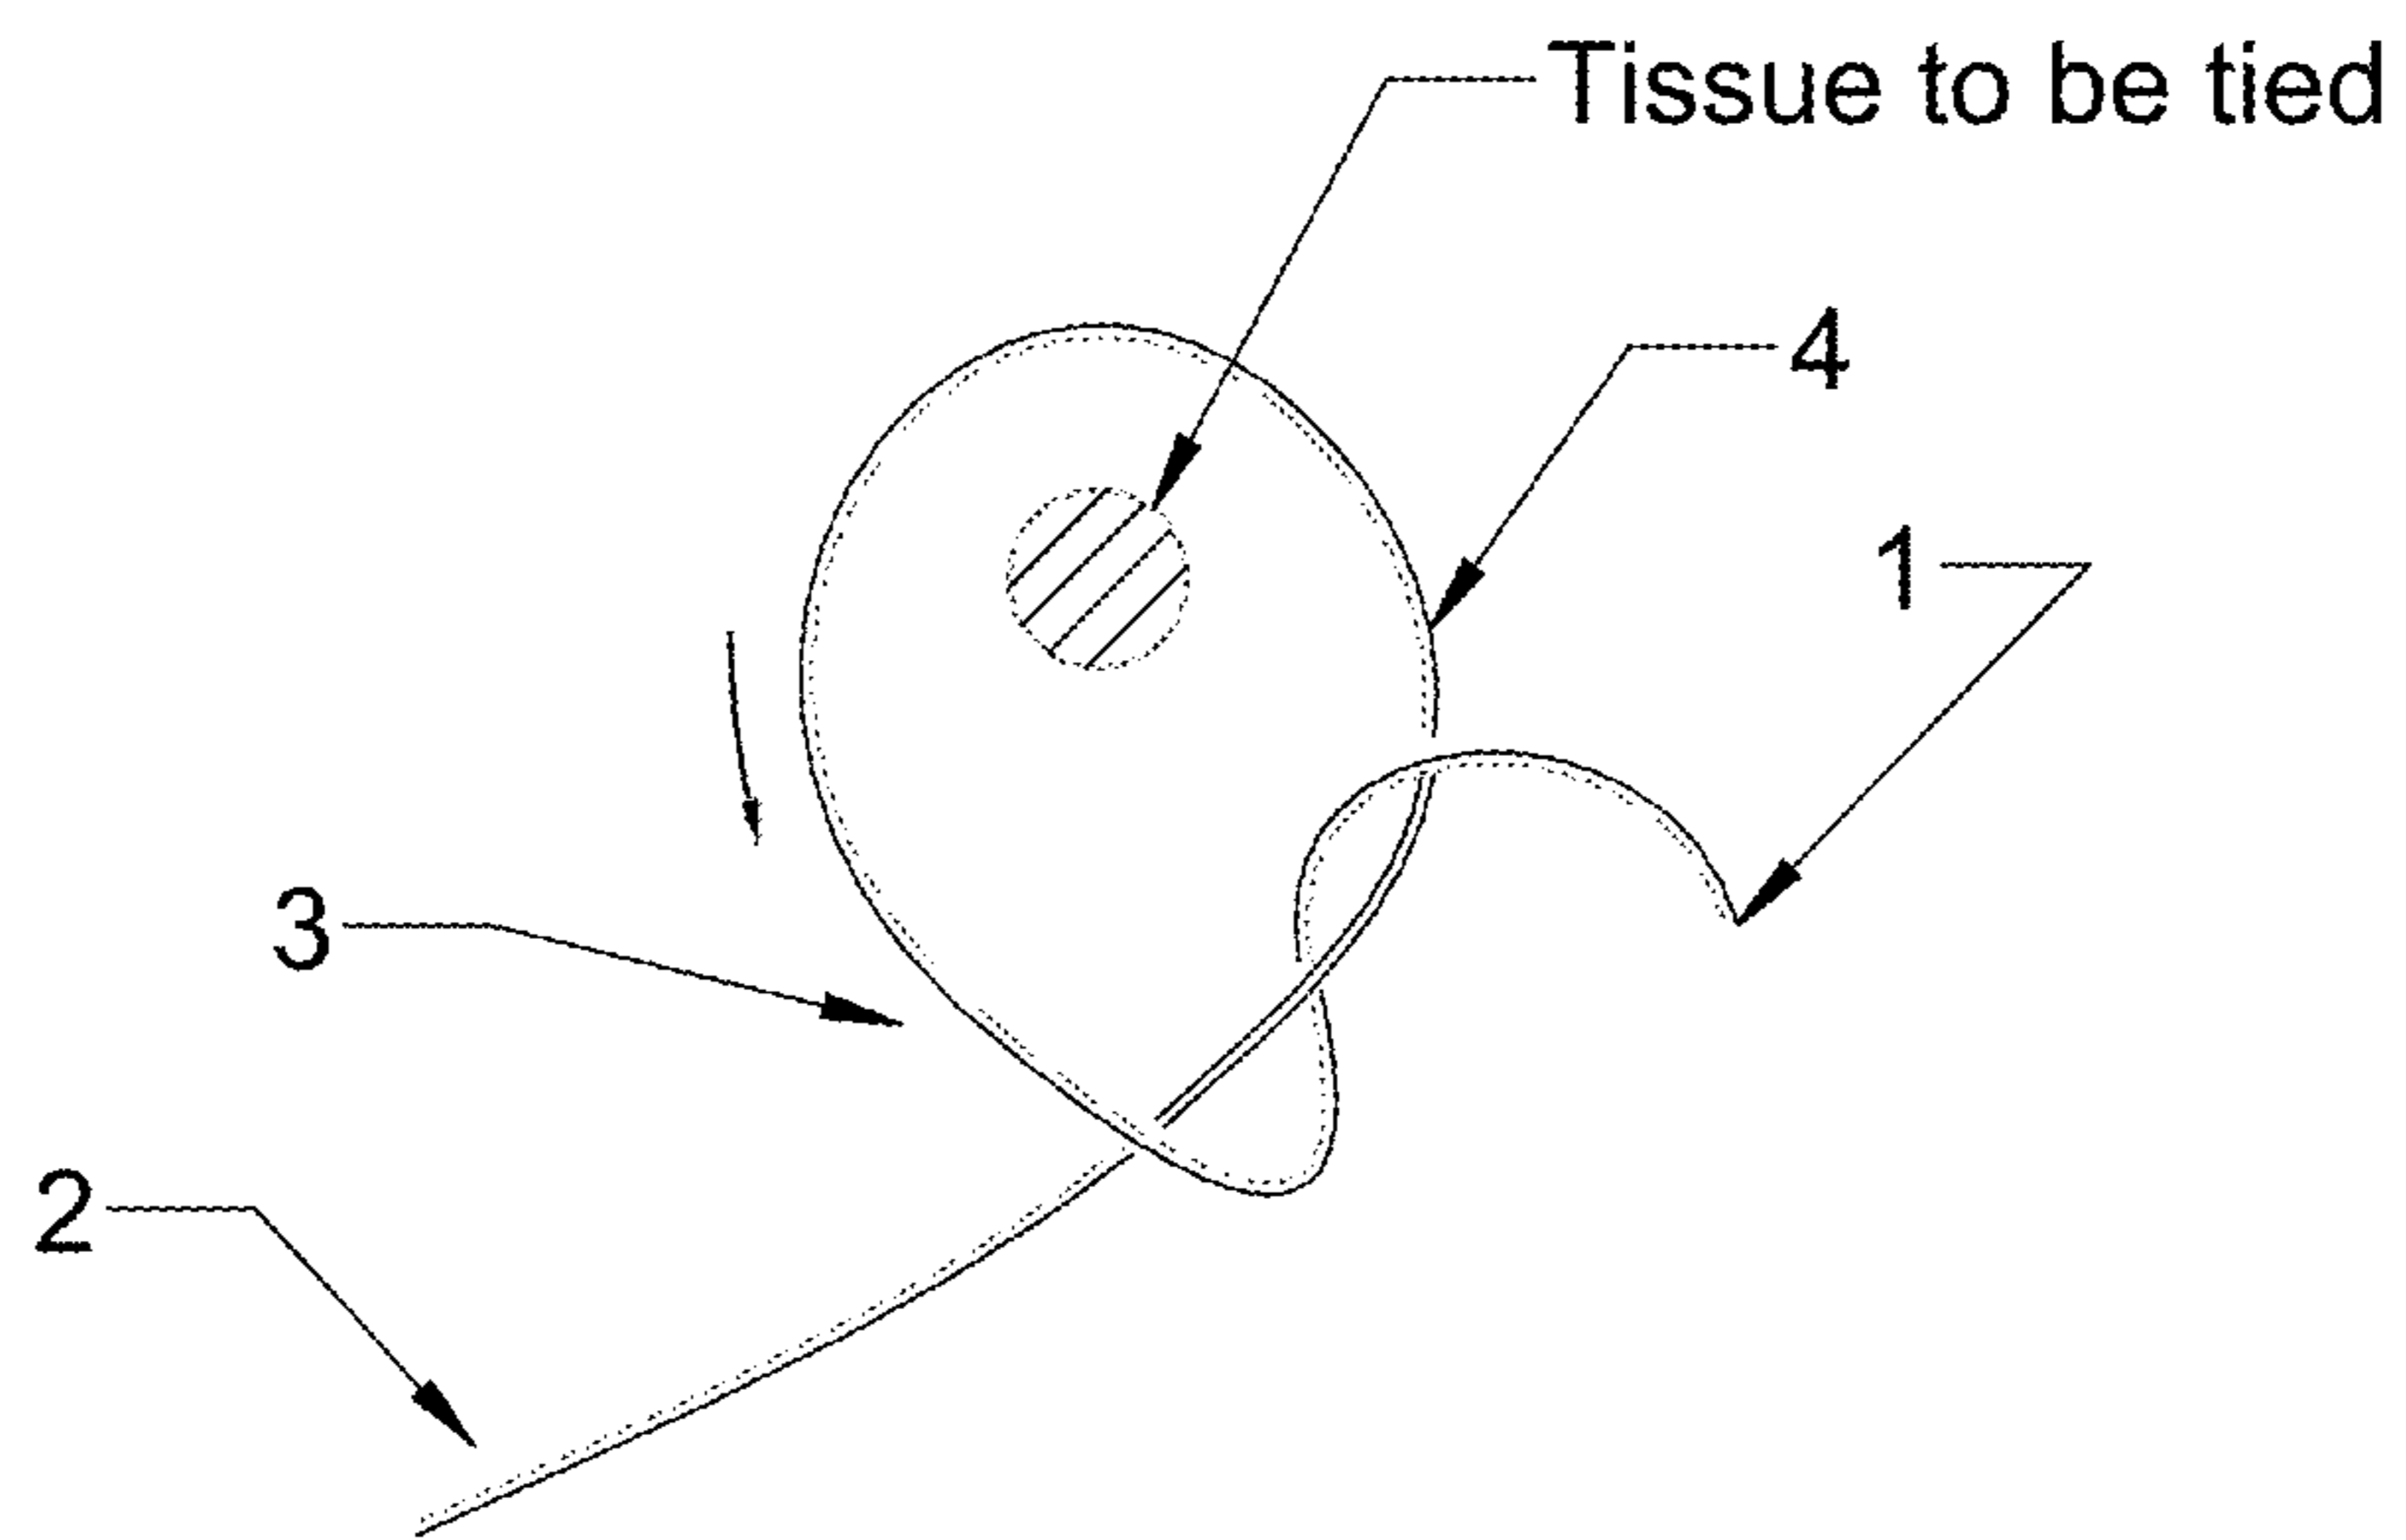


Fig. 60

PRIOR ART

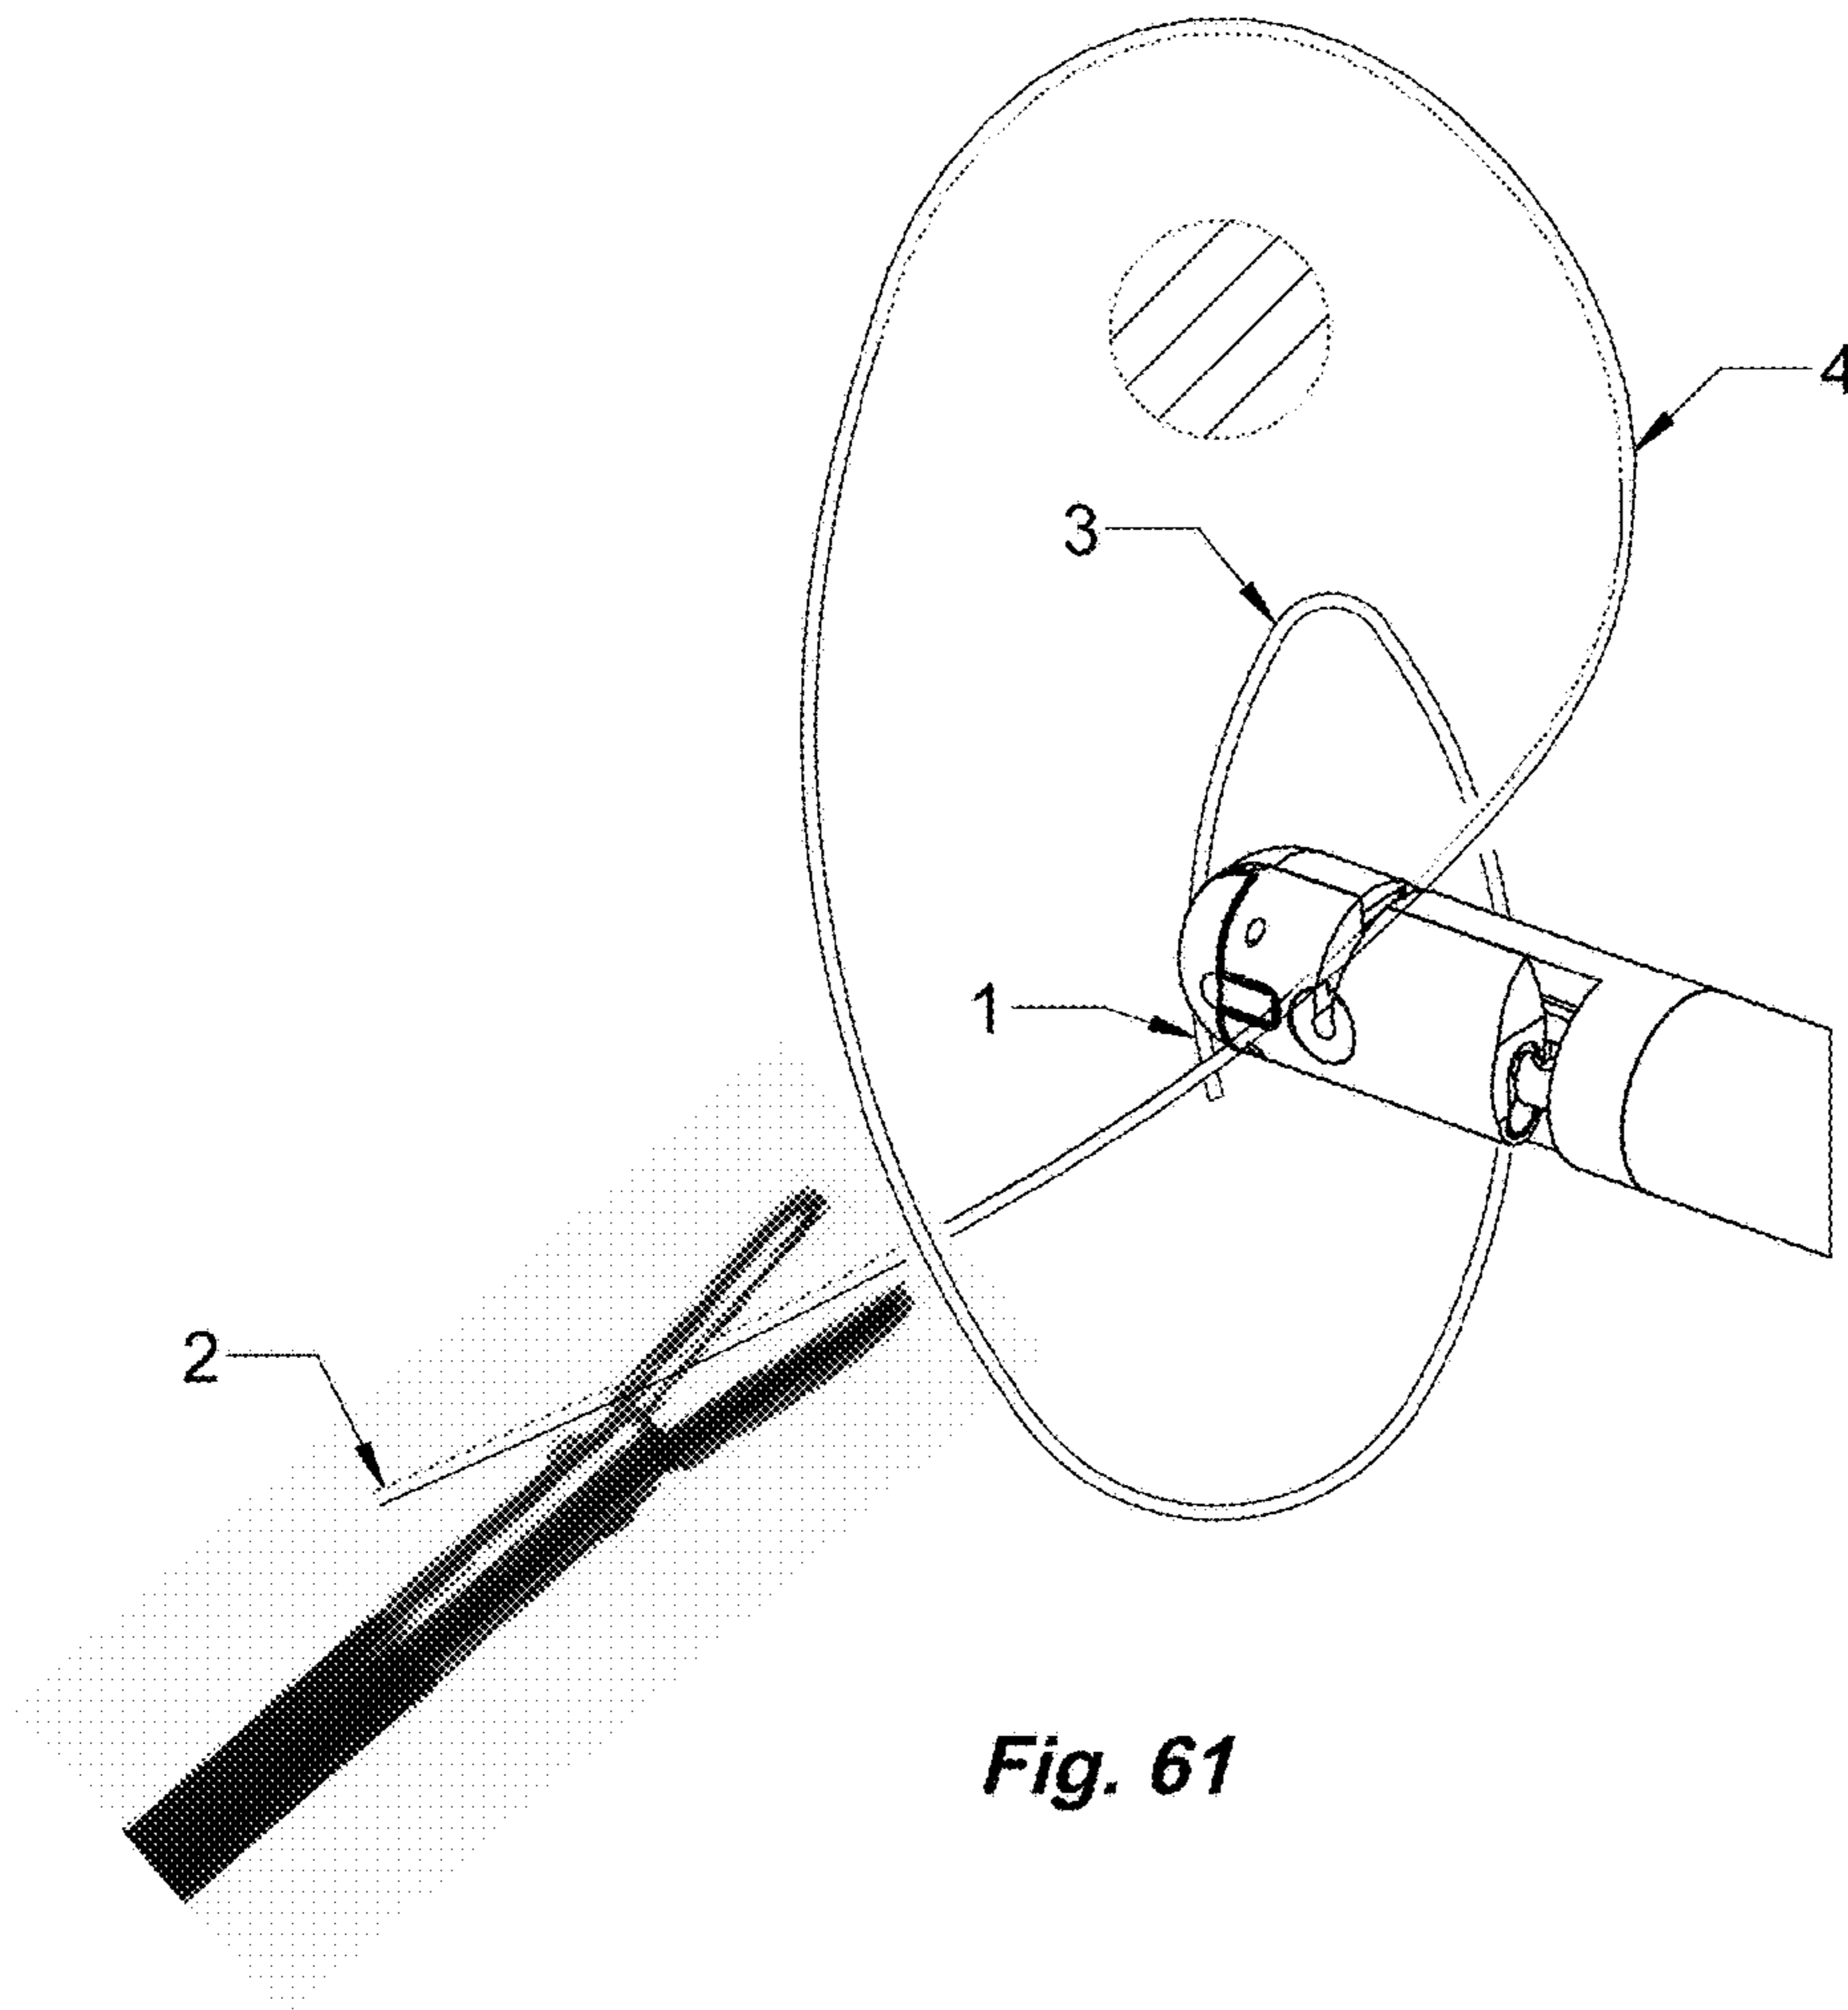


Fig. 61

AUTOMATIC LAPAROSCOPIC KNOT TYING INSTRUMENT

FIELD OF THE INVENTION

A laparoscopic surgical instrument for intra-corporeal knot tying which makes the throw automatically on a free strand of suture ligature, and avoids using the pass or the loop, or having one end of the suture attached to a needle, disc or cartridge. It may be adapted for use in open surgery in deep cavities where the fingers cannot reach, or for use by the robot.

BACKGROUND OF THE INVENTION

Tying of knots is essential in any kind of surgery. It is relatively easy in open surgery, but is difficult in laparoscopic surgery. The current art of laparoscopic knot tying employs either the extra-corporeal method, involving tying the knot by hand outside the body and pushing the knot inside with a knot pusher, or the intra-corporeal method, involving manipulation of the suture with the tips of two laparoscopic graspers, which is cumbersome, and requires considerable skill. Laparoscopic clip applicators, staplers, pre-tied knots and the like are useful substitutes, but cannot totally replace tied knots. Despite considerable prior art, there still is no hand operated instrument that renders laparoscopic intra-corporeal knot tying easier and faster.

In order to describe the tying process, the different parts of the suture ligature need to be given names. As shown in FIG. 59 in the drawings, after the suture ligature has passed around the tissue to be tied, it then presents with a head end (1), a tail end (2), a leading strand (3) and a tail strand (4),

There are two basic methods of tying a knot, whether done openly or laparoscopically. One method is making a “throw” which involves passing the head end of the suture around its tail strand. This is quite simple when performed with the fingers as in tying shoe laces. It does however involve a critical step which is the passing or release and re-grab of the head end of the suture, and wrapping it around the tail strand. In laparoscopic surgery this is difficult because the graspers are trapped in the abdominal wall, and the surgeon is limited to using only two laparoscopic graspers, one in each hand. Hence the reason for the present invention.

The second method of tying a knot involves making a loop or loops, which is commonly performed in open surgery by the surgeon making “instrument ties”, where he uses a needle holder and wraps the suture several times around it. This can be done laparoscopically but is generally difficult. There are many patents in the prior art that try to make the loop laparoscopically, but none has been commercially successful, and this is not the object of the present invention.

the present invention makes the knot differently and automatically without making the loop, or making the pass. Additionally it ties a knot in a free strand of suture ligature, without having one end of the suture being pre-fixed on to a disc or cartridge. It is therefore different in design and technique compared with other previous similar inventions.

Referring to the prior art, the Christoudias Double Grasper has 3 jaws, with a common middle jaw, and functions as a tissue approximator. Its spring loaded actuators are operated by two push buttons. The Ferzli Double Grasper, has a second pair of jaws positioned more proximally on the main shaft, whose purpose is to anchor one end of the suture prior to twisting it around the shaft of the

instrument in order to produce a loop. The Hasson Suture Tying Forceps, is similar to the Ferzli, with 3 finger loops. The orthopedic suture passers are for passing sutures only through hard tissue, and these include the Arthrex Scorpion Suture Passer, and the Arthrex Birdbeak Suture Passer. Some suture passers are for passing sutures through a thickness of soft tissue such as the abdominal wall, and these include the Goretex and the Aesculap. There are devices which “pass the suture-needle” side to side, for inserting sutures into tissues, as well as for tying knots, e.g. the Autosuture’s Endo-stitch, and the Japanese Maniceps. Note these only pass the suture needle, not the suture thread per se. There have been devices that attempt to “automatically” tie a knot, such as Jerrigan’s experimental rotating slotted disc designed for robotic endo-cardiac surgery, but it was abandoned because of the requirement for a cartridge. There have been many devices that help to “create a loop”, with each functioning differently—(a) Kitano’s grasper with the rotating sleeve, Japanese, (b) Donald Murphy’s grasper with the extra horn, Australian, (c) Grice’s sleeve catching instrument, (d) Bagnato & Wilson’s device which simulates the radiological pig-tail catheter, with a preformed loop built into the tip of the catheter, which is deformable and purportedly a loop former, but it is difficult to manufacture and apply, and has not yet been reduced to practice, (e) Ferzli’s double grasper, which anchors one end of the suture, as described above. There have been devices using a “pre-formed knot”, (1) Ethicon’s Endo-Loop, (2) the Duraknot, (3) LSI’s device, (4) Pare’s pre-tied knot, all of which do not help to tie knots.

Past inventions related to intra-corporeal laparoscopic knot tying fail to address the basic problem of “how to make the throw”. They usually offer various alternatives, such as making multiple loops, similar to fishing knots, using pre-tied knots, knot pushers, suture clips, cinchers, tissue fasteners, anchors, stapling devices, etc. The present invention however will assist in manual intra-corporeal knot tying, and will help to produce the knot automatically.

U.S. PATENT DOCUMENTS

1.	3,834,395	Sept. 10, 1974	Manuel Santos	128/326
2.	5,201,759	Apr. 13, 1993	George Ferzli.	606/139
3.	5,217,471	Jun. 8, 1993	Stephen Burkhart	606/148
4.	5,234,443	Aug. 10, 1993	Phan & Stoller	606/148
5.	5,250,054	Oct. 5, 1993	Lehmann Li	606/148
6.	5,281,236	Jan. 25, 1994	Bagnato et al.	606/139
7.	5,312,423	May 17, 1994	Rosenbluth & Brenneman	606/148
8.	5,395,382	Mar. 7, 1995	DiGiovanni et al.	606/148
9.	5,437,682	Aug. 1, 1995	Drew Grice	606/148
10.	5,423,836	Jun. 13, 1995	Scott Brown	606/148
11.	5,439,467	Aug. 8, 1995	Theodore Benderev, et al.	606/139
12.	5,480,406	Jan. 2, 1996	Nolan et al.	606/139
13.	5,728,109	Mar. 17, 1998	Schulze et al.	606/148
14.	5,810,852	Sept. 22, 1998	Greenberg et al.	606/148
15.	5,814,054	Sept. 29, 1998	Kortenbach et al.	606/139
16.	5,846,254	Dec. 8, 1998	Schulze et al.	606/228
17.	6,051,006	Apr. 18, 2000	Shluzas & Sikora	606/148
18.	6,086,601	Jul. 1, 2000	InBae Yoon	606/148
19.	6,221,084	Apr. 24, 2001	R. Fleenor, Pare Surgical	606/148
20.	6,432,118	Aug. 13, 2002	Mollenhauer & Kucklick	606/148
21.	6,716,224	Apr. 26, 2004	Singhatat	606/148
22.	2009/0228025	Sept. 10, 2009	Steven Benson	606/144
23.	2010/0016883	Jan. 21, 2010	George Christoudias	606/205
23.	5,312,423	May 17, 1994	Rosenbluth et al.	606/148
25.	8,512,362	Aug. 20, 2013	Ewers et al.	606/158

OTHER PUBLICATIONS

1. Endo-stitch—Autosuture—Manufacturer’s item #173016.

2. Maniceps—Japanese suturing device, similar to Endo-stitch.
 3. A Laparoscopic Device for Minimally Invasive Cardiac Surg (rotating slotted disc). Shaphan Jernigan, et. al. —European J. of Cardio-thoracic Surgery, Vol. 37, p.626-630. March 2010.
 4. Knot Tying Intra-corporeally, with newly designed Forceps. (sliding sleeve).
 5. Kitano et. al.—J. of Minimal Invasive Therapy & Allied Tech, 1996. 5: 27-28.
 6. Endoscopic Knot Tying Made Easier—(one jaw with extra bump).
 7. Donald Murphy—ANZ J. Surg. 1995. 65, 507-509.
 8. The Excalibur Suturing Needle Holder—(jaw with prominent heel, helps looping)
 9. Uchida et. al. Surgical Endoscopy—vol. 3, 531-532
 10. Aljizawi laparoscopic auto-knot device—(two dissolving balls).
 11. A New Reusable Instrument designed for simple and secure knot tying in laparoscopic surgery. S. S. Miller 1996 Surg. Endos 10: 940-941 (pointed canula).
 12. The Nobel Automatic Laparoscopic Knotting and Suturing Device. Mishra et. al. World Laparoscopy Hospital, India. (a knot pusher)
 13. Automated Knot Tying for Fixation in Minimally Invasive Robot Assisted Cardiac Surgery. March 9(1):105-12.
 14. Kuniholm & Buckner—J. Biomed Eng. November 2005, Vol. 127, 1001-8. JSLS. Jan. 17, 2005.
 15. M I Frecke—Laparoscopic multifunctional instruments: design and testing. Endosc Surg Allied Technol. 1994 December; 2(6):318-9.
 16. G. Berci—Multifunctional laparoscopic Instruments.
 17. <http://www.ligasure.com/ligasure/pages.aspx?page=Products/Laparoscopy>
 18. <http://www.freepatentsonline.com/y2010/0063437>.
 19. <http://www.ncbi.nlm.nih.gov/pubmed/15791983> Multifunctional Laparoscopic Instruments.
- SUGGESTED U.S. CLASSIFICATION: 606/139, 144, 145, 148.
- SUGGESTED INTERNATIONAL CLASSIFICATION: A61B 17/00, 04, 28.
- FIELD OF SEARCH: 606/139, 144, 145, 147, 148, 150, 151, 127, 128, 606/167, 168, 170, 174, 182, 185, 205, 207, 210, 211.
- RELATED PRIOR PATENT: U.S. Pat. No. 9,194,468.

SUMMARY OF THE INVENTION

In laparoscopic surgery, the advent of laparoscopic clips and staples has been a great blessing to surgeons, but cannot totally replace the use of tied knots, which when performed intra-corporeally, is technically difficult, but still necessary. The instrument presented here is intended to facilitate intra-corporeal laparoscopic knot tying with a free strand of suture ligature. It conforms to the customary shape and size of a laparoscopic instrument, with an elongated round sheath, a pistol shaped handle at the proximal end, and a bullet shaped tip at the distal end. Three operating mechanisms are incorporated in the tip: firstly, a grasping mechanism involving the use of a mini-grasper, which is small enough to be contained inside an element that rotates, called the rotator; secondly, a trapping mechanism involving the use of a slotted hollow axle which is an axle with a hollow center, and also involving the use of an open-ended slot on the side of each member of the rotating mechanism, which enables a portion of the tail end of the suture to be trapped within the hollow center, whilst the rotation takes place; thirdly, a

finger activated rotation system, which uses a slider-crank mechanism to convert linear into rotary motion, and uses a patented L-shaped connecting rod to avoid dead centers, and also uses a slotted driven spur gear to transmit the rotation to the slotted rotator, which houses the mini-grasper.

Other characteristics of this instrument include: (1) manipulating both ends of the same suture with the same instrument, (2) being hand operated, avoiding the use of electricity or battery, (3) may be used with a robot, (4) may be used to tie knots in any deep and narrow cavity where the surgeon's fingers cannot reach, (5) allowing the surgeon to tie a knot laparoscopically and automatically, using only his own two hands, without need for help from an assistant.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is perspective view of the entire device from the right side, and

FIG. 2 is the entire device from the left side.

FIG. 3 is a transparent view of the left side of the handle, and

FIG. 4 is the same of the right side of the handle, showing the arrangement of the triggers.

FIG. 5 is a perspective view of the right side of the tip of the instrument, and

FIG. 6 is the left side of the tip, showing the different appearances of the two sides.

FIG. 7 is an exploded view of the handle-assembly from the left side, showing the numerous components within the handle,

FIG. 8 is a perspective view of the handle from the right side, and

FIG. 9 is the handle from the left side, showing the different features on the two sides.

FIG. 10 is a perspective view of the long connector to the trigger of the rotating system and

FIG. 11 is a perspective view of the trigger of this system.

FIG. 12 is a perspective view of the short connector of the grasper rod system.

FIG. 13 is a perspective view of the trigger of the grasper rod system.

FIG. 14 is a view of the thumb push knob.

FIG. 15 shows the long compression spring of the trigger of the rotation system;

FIG. 16 shows the short compression spring of the trigger of the grasper rod system; and

FIG. 17 shows the lid that covers the cavity on the left side the handle.

FIG. 18 shows the external sheath that covers the two rods.

FIG. 19 shows the proximal spacer, which bears two channels.

FIG. 20 shows push rod of the grasper system.

FIG. 21 shows pull rod extension of the rotation system.

FIG. 22 is a perspective view of the tip-assembly, whilst FIG. 23 is an exploded view of the tip-assembly.

FIG. 24 is a top view of the tip-base; and

FIG. 25 is a perspective view of the tip-base,

FIG. 26 is a perspective view of the slotted hollow axle. FIG. 27 shows one of the 3 pins that holds the slotted driven spur gear.

FIG. 28 is a picture of the driven slotted spur gear.

FIG. 29 is a picture of the shoulder screw that holds the driving spur gear.

FIG. 30 is a picture of the driving spur gear.

FIG. 31 is a perspective view of the gear rod.

5

FIG. 32 is a perspective view of the L-shaped connecting rod.

FIGS. 33 and 34 show the shoulder screws used at the ends of the L-rod.

FIG. 35 is a perspective view of the rotator sub-assembly, with the upper jaw closed.

FIG. 36 is the same with the upper jaw open and

FIG. 37 is an exploded view of the same.

FIG. 38 is a perspective view of rotator itself, showing its front end.

FIG. 39 is a perspective view of the same showing its rear end.

FIG. 40 is a perspective view of the upper jaw.

FIG. 41 is a view of the pin that acts as the fulcrum for the upper jaw;

FIG. 42 is a view of the pin that moves the upper jaw.

FIGS. 43, 44 and 45 show 3 of the components of the jaw sub-assembly that moves the upper jaw.

FIG. 46 is a side view of the entire jaw sub-assembly;

FIG. 47 is a top view of the jaw sub-assembly.

FIG. 48 is a picture of the ball with the stem.

FIG. 49 is a perspective view of the oval plate located at the top of the rotator.

FIG. 50 and FIG. 51 are perspective views of the socket that contains the ball.

FIGS. 52, 53, 54, and 55, show the different positions of the rotator during its 360 degree rotation.

FIGS. 56, 57 and 58 show the order of assembly of the major sub-assemblies of the device.

FIG. 59 is diagram indicating the names of the different parts of a suture ligature.

FIG. 60 is diagram showing how a standard throw is formed.

FIG. 61 is a diagram showing the current device being used in conjunction with a regular grasper to tie knot.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

The invention here deploys the following steps in tying a knot: First, the head end of the strand is grasped by a miniature grasper, FIG. 35. Second, the tail strand is temporarily trapped and controlled inside a slotted tubular structure, part 20, FIG. 26.

Third, the miniature grasper which is holding the head end of the suture, is made to rotate 360 degrees around the trapped tail strand, which subsequently escapes from the entrapment, resulting in a tie. In essence, the process requires the tail strand to be temporarily constrained in space, whilst the head end of the suture rotates around it.

The trapping in this device is accomplished by using a slotted hollow axle, part 20, FIG. 26, which is an axle with a hollow center, and also a narrow slot along its entire side. The opening of the slot, 143 allows the tail strand to enter into the hollow space in the center of the axle, 142 and subsequently to escape from it.

In order for the rotation of the head end of the suture to occur whilst the tail strand is trapped, the hollow center and the open side slot are also required in all the other components of the rotation system: the base of the tip, 14, to which the slotted hollow axle is attached, the driven spur gear 17, and the rotator 15, which bears the mini-grasper. This arrangement is necessary for the temporary entrapment and subsequent escape of the tail strand of the suture, as well as the rotation of the rotator. To function well, the slots in all these 4 components must line up precisely during trapping

6

and release of the tail strand of the suture, and at rest, and at the end of a 360 degree rotation.

The crossing-over of the head strand over the tail strand comes about naturally because the strand that is trapped lies at 90 degrees from the strand that rotates.

Rotation is provided by a hand operated slider-crank mechanism that converts the linear motion of a finger pull into a rotational motion, which is then transmitted through the two spur gears to a rotator. The rotator 15 is bonded to the slotted driven spur gear 17, and both have a hollow center and an open slot, like the slotted hollow axle. Both rotate as a unit upon the stationary slotted hollow axle 20, and the minigrasper also rotates with them. The slider-crank mechanism uses an L-shaped connecting rod 21, with two deflecting pillars 134 and 135, to overcome dead centers, which is simpler than using other means such as auxiliary rods. For a description and an explanation of the L-shaped connecting rod, reference is made to U.S. Pat. No. 9,194, 468, by the author. The slider-crank first rotates a driving spur gear 18, then a slotted driven spur gear 17, then a slotted rotator 15, which carries the mini-grasper

The source of energy used for the rotation is a manual pull, with the return being performed automatically by a compression spring. The use of this simple mechanism avoids the use of complicated mechanisms or the use of electricity or the battery.

The mini-grasper sub-assembly, FIG. 35, 36, 37, is essentially a very short laparoscopic grasper, with one movable jaw, but no handle, and no shaft. The minigrasper is spring loaded, and is housed inside the rotator, which rotates on the slotted hollow axle. The mini-grasper is uniquely small and short, but fully functional. In order for it to rotate, its shaft needs to be separated from the long control rod, and it needs to be small enough to fit inside the rotator. The mini-grasper has only a movable upper jaw 16, which is normally held in a closed position by a compression spring, 32.

To grasp a suture the upper jaw 16 needs to be opened by external pressure on the compression spring 32, exerted from the separated control rod, which is initiated by pushing the thumb knob 9, with the thumb at the handle. A special inter-connecting ball and socket joint, FIG. 48, 49, 50, 51, in the control rod allows the rotator with the mini-grasper, to undergo 360 degree rotation in the sagittal plane of the long axis of the instrument, whilst also permitting the jaws to be remotely controlled from the handle with the push or pull, when the rotator is in the resting neutral position.

After the head end of the suture has been grasped by the mini-grasper, the rotation is activated by the index finger pulling on the trigger 4, which causes the slider-crank mechanism to generate the first half of a rotation. The second half of the rotation is generated by a compression spring, when the trigger 4 is released, and is thus automatic.

After the rotator has completed a full rotation, it may be necessary to pull the suture ends apart to tighten the knot. At this point, because the force of the spring in the mini-grasper holding the suture is of limited strength, additional pressure will need to be applied to the upper jaw to hold on to the suture. This is provided by the trigger 3, also operated by the index finger, whose additional pull will help to provide additional pressure keeping the jaw tightly closed holding on to the suture. The separated grasper rod is therefore provided with both a push as well as a pull activation. The push activation is provided by the thumb, whilst the pull activation is provided by the compression spring as well as by the index finger. There is no problem in using the index finger for two different activations since the two are not used simultaneously.

Referring to FIG. 7, the exploded view of the handle sub-assembly, part **1** is a pistol shaped handle which is gripped by the palm and by the middle, ring and little fingers through the loop, whilst freeing the index finger and the thumb for actuation.

The lower trigger is primarily pulled by the index finger. The upper trigger is primarily pushed by the thumb. The return movement on both triggers is performed by compression springs, which are hidden inside the handle. The upper trigger may in addition be pulled by the index finger. The connectors connecting the triggers to the actuating rods are located inside a cavity in the rear of the upper part of the handle.

Part **2** is the proximal spacer, which contains two holes for holding the two rods in place and allows their free passage, and contains a flange to prevent its accidental migration inside the sheath. There is no separate distal spacer which does exist in the rear of the base of the tip. Part **3** is the upper trigger, which is to be pushed forward by the thumb through the push knob, but can also be actively pulled back by the index finger. Part **4** is the lower trigger, which is pulled by the index finger to activate the rotation.

Both part **3** and part **4** triggers consist of a 9.5 mm diameter button at the outer end, an intermediate 5 mm diameter rod, and an inner 3 mm diameter rod, which screws into the lower end of the respective connectors further described below. Part **5** is the short connector whose upper end receives the flat neck of the proximal end of the push rod, and its lower end receives the upper trigger. Part **6** is the longer connector whose upper end receives the circular neck of the proximal end of the pull rod, and its lower end receives the lower trigger. Part **7** is a short compression spring used with the upper trigger. Part **8** is a long compression spring used with the lower trigger. Part **9** is the thumb push knob which screws into the upper (push/pull) trigger rod used for opening and closing the movable upper jaw of the mini-grasper. Part **10** is the lid for covering up the cavity on the left side of the handle, containing the connectors. FIG. **8** illustrates **101** which refers to the finger loop, **102** refers to the space inside the finger loop. **103** refers to the seating for trigger for the rotary system, whilst **104** refers to the seating of the trigger for the grasper system. **105** is an empty space, to lighten the weight of the handle. FIG. **9** illustrates the handle from the left side, showing different features **106** and **107**.

FIG. **10** is a perspective view of the long connector to the trigger of the rotating system and FIG. **11** is a perspective view of the trigger of this system. **108** shows the seating for the head end of the rod, **109** shows the seating for the flat neck of the rod. **111** is the male threaded end which screws into the hole **110**. **112** is the 3 mm diameter portion of the shaft of the trigger, over which the compression spring is installed. **113** is a shoulder stop. **114** is the external button. FIG. **12** is a perspective view of the short connector of the grasper rod system, which is similar to FIG. **10**. **109** is the slot that receives the flat neck of the rod. FIG. **13** is a perspective view of the trigger of the grasper rod system, showing **115** which is a female threaded hole, receiving **117** of part **9**. FIG. **14** is a view of the thumb lush knob **116** of the grasper rod system. FIG. **15** shows the long compression spring of the trigger of the rotation system; FIG. **16** shows the short compression spring of the trigger of the grasper rod system; and FIG. **17** shows the lid that covers the cavity on the left side the handle. FIG. **18** shows the external sheath that covers the two rods. FIG. **19** shows the proximal spacer, which bears two channels, **118** and **119**, for supporting the

two rods and keeping them aligned. Its rear flange **120** is to prevent accidental migration into the rear of the sheath.

FIG. **20** shows part **12**, the 2.5 mm push rod of the grasper system, whose proximal end, **122** bears a narrow flat sided neck which mates into the top of the short connector, and helps to prevent accidental rotation of the rod. Its distal end **121** is mated to the socket holding the ball, which is part of a ball and socket joint, which in turn is part of the actuator that moves the upper jaw.

FIG. **21** shows part **13**, the 3 mm pull rod extension of the rotation system with the narrow flat neck, **124**, whose distal end **123**, screws into the proximal end of the "gear rod" part **9**, and whose proximal end has a round cut out to create a narrow round neck, to mate with the top of the long connector.

FIG. **22** is a perspective view of the tip sub-assembly, whilst FIG. **23** is an exploded view of the same, showing the numerous components. Part **14** is the tip-base, without the rotator, and houses the components of the rotational mechanism, which include the crank-slider, the L-shaped connecting rod, the deflecting pillars, the driving spur gear, and the driven spur gear, and provides the base for fixation of the slotted hollow axle. It also bears a V-shaped slot on its side for guiding the tail end of the suture into the trap. This slot may be located alternately at the very tip of the base. Part **15** is the rotator, which is a complex and crucial body, representing a short sagittal portion of the tip, and participates in each of the trapping, grasping and rotating mechanisms. Part **16** is the movable upper jaw. Part **18** is the driving spur gear, which bears a counter sunk hole in the center for mounting a shoulder screw, and a smaller screw in its periphery for mounting the distal end of the L-shaped connecting rod. Its origin is identical to the slotted driven gear, so their teeth can match. Part **17** is the slotted driven spur gear, which is similar to part **18**, but has an open slot between two adjacent teeth, allowing access to the hollow space in the center. This is part of the trapping mechanism. Its upper surface is fixed to the underside of the rotator, either by adhesives or by 3 tiny pins, through 3 tiny counter-sunk holes. It is designed intentionally with a small number of teeth, in order to create a wide enough slot between two adjacent teeth, for the suture to pass through. The gap created between two adjacent teeth on the other hand must not damage the teeth. Part **19** is the shoulder screw for mounting the driving spur gear. Part **20** is the slotted hollow axle, which bears a male thread at one end, a retaining flange at the other end, a hollow center throughout its length, and an open ended slot on the entire length of its side. Part **20** is the slotted hollow axle, which screws into the base of the tip, **126**. Part **15** is the rotator that rotates upon the flat platform **125** of the tip base. Part **16** is the upper jaw. The lower jaw is an integral part of the rotator. The hollow center is for temporary trapping of a portion of the suture, and the slot of the side is provide entry and exit for the suture. Part **21** is the L-shaped connecting rod which is a flat structure, with its side arm installed proximally, and connected to the round gear rod **25**. Part **22** is the screw that attaches the distal end of the connecting rod to the periphery of the driving spur gear. Part **23** is the screw that attaches the proximal end of the L-connecting rod to the gear rod. Part **24** is the socket that houses the ball attached to the rotator. Part **25** is the push/pull rod whose distal end is attached to the upper end of the socket, and whose proximal end is attached to the short connector. Part **14** is the large base of the tip.

Referring to FIG. **24** and FIG. **25**, concerning the tip base, **126** is a female threaded hole that receives the male thread of the slotted hollow axle, **20** and illustrates element **130**.

127 receives the mounting shoulder screw of the driving spur gear. **128** is a shoulder stop for the distal end of the sheath. **129** is the channel in which the gear rod **25** travels. **131** is the seat for the slotted driven spur gear. **132** is the v-shaped slot for the tail strand to slide in and out. **133** is the seat for the driving spur gear. **134** and **135** are the deflecting pillars, which are strategically located, so that they will deflect the distal end of the connecting rod off the dead center positions, just before the end of the travel of the side arm in either direction. **136** is the end of channel **129**, for the gear rod to slide up and down. **137** and **138** are channels which guide the grasper rod. **139** is the end of an elliptical cut out which extends from the upper edge of the platform **125** to the upper end of the tip base. This space allows the L-shaped connecting rod to operate.

FIG. **26** is a perspective view of the slotted hollow axle, part **20** and illustrates element **140**. **141** is the retaining flange. **142** is the hollow center. **143** is the open slot that extends through the entire length of the axle. **144** is the male thread. FIG. **27** shows one of the 3 pins that holds the slotted driven spur gear through **148** to underside of the rotator. FIG. **28** is a picture of the driven slotted spur gear. **145** shows the width of the gap between two adjacent teeth, which is vital for creating the slot **147**. **146** is the central hole for mounting the part **20**. FIG. **29** is a picture of the shoulder screw that holds the driving spur gear. FIG. **30** is a picture of the driving spur gear, showing the holes **149** and **150** for the mounting screw with counter-sunk head. **151** is a hole for a miniature screw that joins the driving spur gear to the hole **154** of the L-rod. FIG. **31** is a perspective view of the gear rod, which bears a female hole **152**, on the side near its distal end, for attachment to **158** of the L-rod, and bears a female hole **153** on its proximal end for joining to the rod extension. FIG. **32** is a perspective view of the L-shaped connecting rod, whose proximal end **158** is attached to **152** of the gear rod, and whose distal end **154** is attached to **151** of the driving spur gear. **156** is the side arm, whose edges **155** and **157**, make contact with the pillars **134** and **135**.

FIG. **37** is an exploded view of the rotator sub-assembly, showing the numerous components. Part **15** is the rotator. Part **16** is the upper jaw. Part **26** is the adaptor with an oval slot on its side for the pin **27** to move up and down, thereby converting vertical motion into horizontal, in moving the upper jaw. Part **27** is the pin that moves the upper jaw. Part **28** is the pin that acts as the fulcrum for moving the upper jaw. Part **29** is the screw that joins the oval plate to the plunger. Part **30** is the oval plate, which acts an adaptor which changes the line of action of the push/pull rod from the midline to the side of the rotator. Part **31** is the plunger, being part of the actuating system of the upper jaw. Part **32** is the compression spring. Part **33** is the stem of the ball. Part **34** is the ball. Part **35** is the socket. Part **36** are the 3 tiny pins for attaching the driven spur gear to the underside of the rotator.

Referring to FIGS. **38** and **39**, concerning the rotator itself, it is a complex and crucial structure. **160** is for the hollow axle, and **159** is for its counter-sunken flange. **161** is for the swinging arm of the upper jaw **173**. **162** is for the fulcrum pin **28**. **163** is the housing for the adaptor **26**. **164** is an intentional groove on the lower jaw. **165** is the fixed lower jaw. **166** is the V-shaped slot for entry/exit of the tail strand of the suture. **167** is for installing the plunger and compression spring. The combination of **167** and **168** is for the oval plate.

FIG. **40** is a perspective view of the upper jaw, part **16**. **169** is the hole for mounting the actuating pin **27**, which

moves the jaw. **170** is for mounting the screw **28** acting as fulcrum for the jaw. **171** is the gripping surface. **172** is the rounded upper surface.

Referring to FIGS. **43** and **44**, the top of the plunger has a female threaded hole **174** for the screw **29** that secures it to the oval plate. **175** is the head of plunger, and **176** is the shaft over which the compression spring rests. **177** is the male threaded end which mates into the female hole **178** on the adaptor **26**. **179** is an oval slot transversely placed on the adaptor which is necessary to compensate for circular path of travel of pin **27** on the upper jaw.

FIGS. **43**, **44** and **45** show 3 of the components of the jaw sub-assembly that moves the upper jaw, including the plunger **31**, the adaptor **26**, and the compression spring **32**.

FIGS. **46** and **47** show the entire jaw sub-assembly. Part **26** is the adaptor with an oval slot placed horizontally on its side. Part **31** is the plunger which screws into the top of the adaptor **26**, with a compression spring **32** mounted on its shaft. On its upper end is mounted the oval adaptor, secured with the screw **29**. On the other end of the oval adaptor is mounted the stem of the ball, in the midline of the rotator, and in line with the socket.

FIG. **48** is a picture of the ball **34** with the stem **33**. FIG. **49** is a perspective view of the oval plate located at the top of the rotator that is responsible for diverting the forces of actuation from the midline to the side of the rotator. **181** and **182** receives the counter-sunk screw. **180** receives the stem of the ball.

FIG. **50** and FIG. **51** are perspective views of the socket that contains the ball, illustrated by elements **183**, **184**. Note the socket is open at the lateral sides allowing the ball to escape and enter at the sides.

Referring to FIGS. **55**, **57**, and **58**, the order of assembly is explained. First the sub-assemblies are constructed, which include the rotator sub-assembly, the tip-base sub-assembly, and the handle sub-assembly. Next the rotator sub-assembly is mounted on the tip-base sub-assembly. Then the two long operating rods are mounted followed by the outer sheath, and the proximal spacer. Next the rear end of this large sub-assembly is carefully inserted into the front of the handle, secured in place, followed by installation of the long and short connectors into the cavity in the handle, followed by installation of the triggers and compression springs.

FIG. **59** is diagram indicating the names of the different parts of a suture ligature, **1** for the head end, **2** the tail end, **3** the leading strand, and **4** the tail strand.

FIG. **61** shows how a knot is made using the present instrument. The tail end of the suture is grasped with a regular grasper, and is pulled taut so that the tail strand becomes relatively taut. The jaw of the mini-grasper then grasps the head end of the suture, and the instrument is pulled back over the tail strand, crossing it. The tail strand is then engaged in the V-slot on the upper surface of the tip of the present instrument, and seated firmly in the central space of the hollow axle. The rotation trigger **4**, is then fired. The rotator will rotate through 180 degrees. Upon release of the rotation trigger, the compression spring will make the rotator rotate through the second 180 degrees, carrying the head end of the suture with it, producing the throw. Pulling the two ends apart will result in a knot. The process may be repeated.

What is claimed:

1. A laparoscopic instrument for intra-corporeal tying of knots with a free strand of a suture-ligature, comprising;
 - a shaft attached to a handle with controls;
 - a bullet shaped tip having a rotator subassembly, tip base subassembly and slider crank mechanism; wherein the

rotator subassembly includes a slotted hollow axle with a hollow center and an open ended slot on its entire side, a mini-grasper with a movable jaw contained within the rotator subassembly and the rotator subassembly is configured to rotate 360 degrees on the hollow axle, along a sagittal plane of the long axis of the instrument; and

wherein the mini-grasper is configured to grasp a head end of a suture, the slotted hollow axle is configured to temporarily trap a tail strand of the suture so that when the rotator subassembly rotates 360 degrees to form a knot in the suture.

2. A method of forming a laparoscopic knot with a free strand of a suture-ligature, comprising;

providing a laparoscopic instrument with a shaft attached to a handle with controls, a bullet shaped tip having a rotator subassembly, tip base subassembly and slider crank mechanism; wherein the rotator subassembly includes a slotted hollow axle with a hollow center and an open ended slot on its entire side, a mini-grasper with a movable jaw contained within the rotator subassembly and the rotator subassembly is configured to rotate 360 degrees on the hollow axle, along a sagittal plane of the long axis of the instrument;

grasping a head end of a suture with the mini-grasper, trapping a tail strand of the suture with the slotted hollow axle,

forming a knot by rotating the rotator subassembly 360 degrees.

* * * * *

30