



US009682373B2

(12) **United States Patent**
Losada et al.

(10) **Patent No.:** **US 9,682,373 B2**
(45) **Date of Patent:** ***Jun. 20, 2017**

(54) **DEVICE FOR SEPARATING COMPONENTS OF A FLUID SAMPLE**

(71) Applicant: **Becton, Dickinson and Company**, Franklin Lakes, NJ (US)

(72) Inventors: **Robert J. Losada**, Astoria, NY (US); **Gregory L. Lusardi**, Hackettstown, NJ (US); **Fu-Chung Lin**, Wayne, NJ (US)

(73) Assignee: **Becton, Dickinson and Company**, Franklin Lakes, NJ (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **13/862,746**

(22) Filed: **Apr. 15, 2013**

(65) **Prior Publication Data**
US 2013/0241099 A1 Sep. 19, 2013

Related U.S. Application Data
(60) Continuation of application No. 13/085,831, filed on Apr. 13, 2011, which is a division of application No. (Continued)

(51) **Int. Cl.**
B01L 3/00 (2006.01)
G01N 33/49 (2006.01)
B04B 7/08 (2006.01)

(52) **U.S. Cl.**
CPC **B01L 3/50215** (2013.01); **B04B 7/08** (2013.01); **G01N 33/491** (2013.01); **Y10T 29/49826** (2015.01)

(58) **Field of Classification Search**
CPC B01D 33/00; B01D 21/26; B01D 17/038; B01D 21/00; B01D 21/262;
(Continued)


(56) **References Cited**
U.S. PATENT DOCUMENTS
2,577,780 A 12/1951 Lockhart
2,693,049 A 11/1954 Atton
(Continued)

FOREIGN PATENT DOCUMENTS
DE 2749130 A1 5/1979
EP 0017127 B1 10/1980
(Continued)

Primary Examiner — Lore Jarrett
(74) *Attorney, Agent, or Firm* — The Webb Law Firm

(57) **ABSTRACT**
A separator for use in a container for a biological fluid is disclosed. The separator includes a separator body having a first region at least partially made of a first material having a first density, and a second region at least partially made of a second material having a second density different from the first density. The separator has an overall density intermediate the densities of a first phase and a second phase of the biological fluid. At least a portion of the separator is deformable between a first condition in which the biological fluid can pass between an inner surface of the container and the separator, and a second condition in which at least a portion of the separator prevents the biological fluid from passing between the inner surface of the container and the separator.

9 Claims, 9 Drawing Sheets

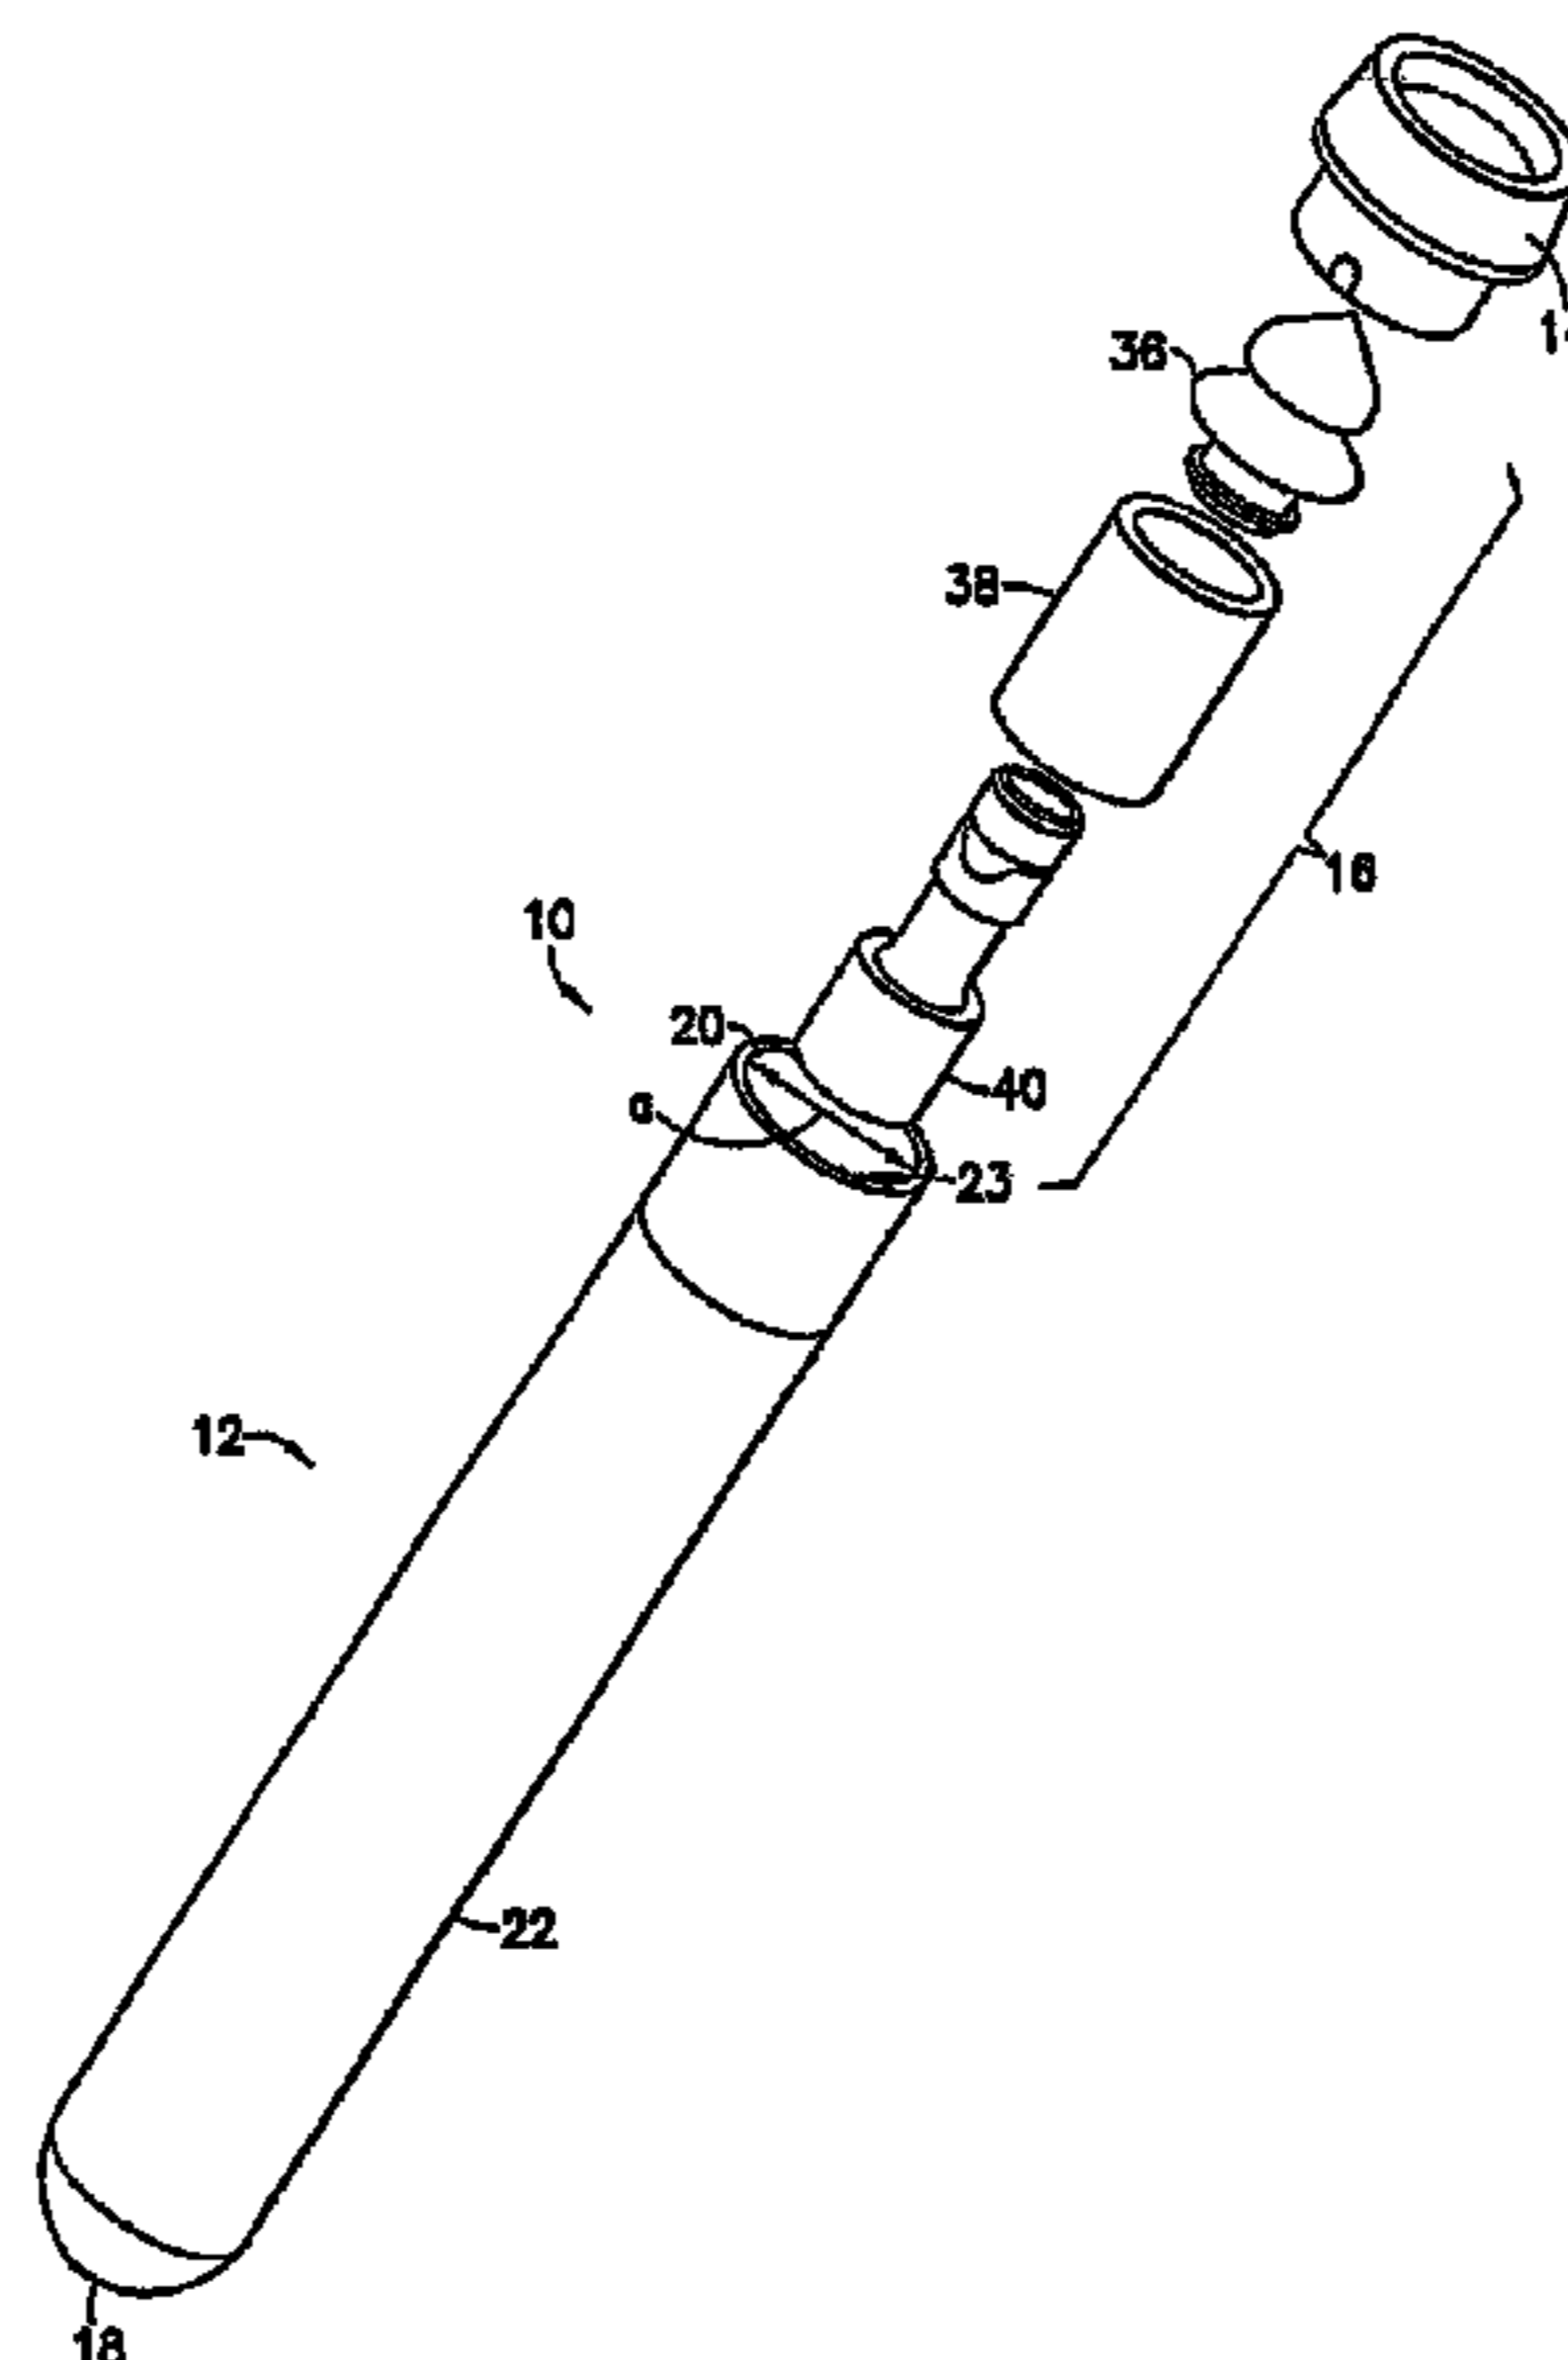

Related U.S. Application Data

10/785,893, filed on Feb. 24, 2004, now Pat. No. 7,947,236, which is a continuation-in-part of application No. 09/727,282, filed on Nov. 30, 2000, now Pat. No. 6,803,022, which is a continuation-in-part of application No. 09/454,988, filed on Dec. 3, 1999, now Pat. No. 6,479,298.

(58) **Field of Classification Search**

CPC B01D 17/0217; G01N 1/18; G01N 33/48; G01N 33/491; B01L 3/50215; B04B 7/08; Y10T 29/49826

See application file for complete search history.

(56)

References Cited

U.S. PATENT DOCUMENTS

2,910,798 A 11/1959 Bias
 3,300,051 A 1/1967 Mitchell
 3,326,215 A 6/1967 Samoff et al.
 3,508,653 A 4/1970 Coleman
 3,647,070 A 3/1972 Adler
 3,654,925 A 4/1972 Holderith
 3,661,265 A 5/1972 Greenspan
 3,741,400 A * 6/1973 Dick B01L 3/5021
 210/516
 3,747,257 A 7/1973 Olsen
 3,771,965 A 11/1973 Grams
 3,779,383 A 12/1973 Ayres
 3,780,935 A 12/1973 Lukacs et al.
 3,786,985 A 1/1974 Blaiivas
 3,800,947 A 4/1974 Smith
 3,809,733 A 5/1974 Sandiford et al.
 3,814,248 A * 6/1974 Lawhead 210/789
 3,814,258 A 6/1974 Ayres
 3,849,072 A 11/1974 Ayres
 3,850,174 A 11/1974 Ayres
 3,852,194 A 12/1974 Zine, Jr.
 3,862,042 A 1/1975 Ayres
 3,879,295 A 4/1975 Glover et al.
 3,882,021 A 5/1975 Ayres
 3,886,928 A 6/1975 Sarstedt
 3,887,464 A 6/1975 Ayres
 3,887,465 A 6/1975 Ayres
 3,887,466 A 6/1975 Ayres
 3,890,237 A 6/1975 Welch
 3,890,954 A 6/1975 Greenspan
 3,891,553 A 6/1975 Ayres
 3,894,950 A 7/1975 Ayres et al.
 3,894,951 A 7/1975 Ayres
 3,894,952 A 7/1975 Ayres
 3,897,337 A 7/1975 Ayres
 3,897,340 A 7/1975 Ayres
 3,897,343 A 7/1975 Ayres
 3,901,219 A 8/1975 Kay
 3,909,419 A 9/1975 Ayres
 3,919,085 A 11/1975 Ayres
 3,920,549 A 11/1975 Gigliello et al.
 3,920,557 A 11/1975 Ayres
 3,929,646 A 12/1975 Adler
 3,931,018 A 1/1976 North, Jr.
 3,932,277 A 1/1976 McDermott et al.
 3,935,113 A 1/1976 Ayres
 3,941,699 A 3/1976 Ayres
 3,945,928 A 3/1976 Ayres
 3,951,801 A 4/1976 Ayres
 3,957,654 A 5/1976 Ayres
 3,960,727 A 6/1976 Hochstrasser
 3,969,250 A 7/1976 Farr
 3,970,565 A 7/1976 Ahlstrand et al.
 3,972,812 A 8/1976 Gresl, Jr.
 3,981,804 A 9/1976 Gigliello
 4,001,122 A 1/1977 Griffin
 4,021,340 A 5/1977 Zine, Jr.
 4,021,352 A 5/1977 Sarstedt
 4,027,660 A 6/1977 Wardlaw et al.

4,055,501 A 10/1977 Cornell
 4,057,499 A 11/1977 Buono
 4,077,396 A 3/1978 Wardlaw et al.
 4,082,085 A 4/1978 Wardlaw et al.
 4,083,788 A 4/1978 Ferrara
 4,088,582 A 5/1978 Murty et al.
 4,119,125 A 10/1978 Elkins
 4,131,549 A 12/1978 Ferrara
 4,134,832 A 1/1979 Heimreid
 4,142,668 A 3/1979 Lee
 4,152,270 A 5/1979 Cornell
 4,154,690 A 5/1979 Ballies
 4,159,896 A 7/1979 Levine et al.
 4,169,060 A 9/1979 Columbus
 4,189,385 A * 2/1980 Greenspan 210/136
 4,202,769 A 5/1980 Greenspan
 4,246,123 A 1/1981 Cornell et al.
 4,257,886 A 3/1981 Kessler
 4,279,863 A 7/1981 Friehter
 4,294,707 A 10/1981 Ikeda et al.
 4,315,892 A 2/1982 Stone et al.
 4,364,832 A 12/1982 Ballies
 4,369,117 A 1/1983 White
 4,379,849 A 4/1983 Heimreid
 4,396,381 A 8/1983 Fanger et al.
 4,409,988 A 10/1983 Greenspan
 4,417,981 A 11/1983 Nugent
 4,425,235 A 1/1984 Cornell et al.
 4,426,290 A 1/1984 Ichikawa et al.
 4,443,345 A 4/1984 Wells
 4,464,254 A 8/1984 Dojki et al.
 4,492,634 A 1/1985 Villa-Real
 4,517,090 A 5/1985 Kersten et al.
 4,522,713 A 6/1985 Nussbaumer et al.
 4,533,474 A 8/1985 Arnaudeau
 4,567,754 A 2/1986 Wardlaw et al.
 4,569,764 A 2/1986 Satchell
 4,602,995 A 7/1986 Cassaday et al.
 4,707,276 A 11/1987 Dodge et al.
 4,770,779 A 9/1988 Ichikawa et al.
 4,818,386 A 4/1989 Burns
 4,828,716 A 5/1989 McEwen et al.
 4,832,851 A 5/1989 Bowers et al.
 4,853,137 A 8/1989 Ersson
 4,877,520 A 10/1989 Burns
 4,917,801 A 4/1990 Luderer et al.
 4,957,637 A 9/1990 Cornell
 5,007,892 A 4/1991 Columbus
 5,019,243 A 5/1991 McEwen et al.
 5,030,341 A 7/1991 McEwen et al.
 5,086,784 A 2/1992 Levine et al.
 5,112,490 A 5/1992 Turpen
 5,171,533 A 12/1992 Fine et al.
 5,236,604 A 8/1993 Fiehler
 5,251,474 A 10/1993 Wardlaw et al.
 5,269,927 A 12/1993 Fiehler
 5,271,852 A 12/1993 Luoma, II
 5,282,981 A 2/1994 Adams et al.
 5,308,506 A 5/1994 McEwen et al.
 5,325,977 A 7/1994 Haynes et al.
 5,354,483 A 10/1994 Furse
 5,389,265 A 2/1995 Luoma, II
 5,393,494 A 2/1995 Greenfield et al.
 5,419,835 A 5/1995 Adams et al.
 5,422,018 A 6/1995 Saunders et al.
 5,454,958 A 10/1995 Fiehler
 5,455,009 A 10/1995 Vogler et al.
 5,456,885 A 10/1995 Coleman et al.
 5,462,716 A 10/1995 Holm
 5,474,687 A 12/1995 Van Vlasselaer
 5,511,558 A 4/1996 Shepard et al.
 5,533,518 A 7/1996 Vogler
 5,552,325 A 9/1996 Nochumson et al.
 5,556,541 A 9/1996 Ruschke
 5,560,830 A 10/1996 Coleman et al.
 5,575,778 A 11/1996 Hardt et al.
 5,577,513 A 11/1996 Van Vlasselaer
 5,632,895 A 5/1997 Tsukagoshi et al.
 5,632,905 A 5/1997 Haynes

(56)

References Cited

U.S. PATENT DOCUMENTS


5,646,004 A 7/1997 Van Vlasselaer
 5,648,223 A 7/1997 Van Vlasselaer
 5,707,876 A 1/1998 Levine
 5,736,033 A 4/1998 Coleman et al.
 5,785,925 A 7/1998 U'Ren
 5,840,502 A 11/1998 Van Vlasselaer
 5,853,600 A 12/1998 McNeal et al.
 5,860,937 A 1/1999 Cohen
 5,955,009 A 9/1999 Kazuma
 6,001,087 A 12/1999 Zurcher
 6,063,297 A 5/2000 Antanavich et al.
 6,074,613 A 6/2000 Harness et al.
 6,074,883 A 6/2000 Kelly et al.
 6,161,712 A 12/2000 Savitz et al.
 6,174,447 B1 1/2001 Spindler
 6,225,123 B1 5/2001 Cohen et al.
 6,277,331 B1 8/2001 Konrad
 6,280,400 B1 8/2001 Niermann
 6,302,919 B1 10/2001 Chambers et al.
 6,390,966 B2 5/2002 Anderson
 6,406,671 B1 6/2002 DiCesare et al.
 6,409,528 B1 6/2002 Bodnar
 6,465,256 B1 10/2002 Iskra
 6,471,069 B2 10/2002 Lin et al.
 6,479,298 B1* 11/2002 Miller et al. 436/177
 6,497,325 B1* 12/2002 DiCesare et al. 210/516
 6,516,953 B1 2/2003 DiCesare et al.
 6,537,503 B1 3/2003 Conway
 6,582,904 B2 6/2003 Dahm
 6,593,145 B2 7/2003 Macfarlane et al.
 6,740,240 B2 5/2004 Coville et al.
 6,758,804 B2 7/2004 Anderson
 6,783,346 B2 8/2004 Bodmer et al.
 6,793,892 B1 9/2004 Niermann
 6,803,022 B2 10/2004 DiCesare et al.
 6,817,256 B2 11/2004 Mehra et al.
 6,979,307 B2 12/2005 Beretta et al.
 7,074,577 B2 7/2006 Haubert et al.
 7,077,273 B2 7/2006 Ellsworth et al.
 7,153,477 B2 12/2006 DiCesare et al.
 7,179,391 B2 2/2007 Leach et al.
 7,205,157 B2 4/2007 Jurgensen et al.
 7,211,433 B1 5/2007 Dahm et al.
 7,220,593 B2 5/2007 Haubert et al.
 7,223,346 B2 5/2007 Dorian et al.
 7,309,468 B2 12/2007 Stevens et al.
 7,329,534 B2 2/2008 Haubert et al.
 7,358,095 B2 4/2008 Haubert et al.
 7,374,678 B2 5/2008 Leach et al.
 7,445,125 B2 11/2008 Ellsworth et al.
 7,470,371 B2 12/2008 Dorian et al.
 7,547,272 B2 6/2009 Ellsworth et al.
 7,578,975 B2 8/2009 DiCesare et al.
 7,629,176 B2 12/2009 Haubert et al.
 7,645,425 B2 1/2010 Haywood et al.
 7,736,593 B2 6/2010 Dastane et al.
 7,745,106 B2 6/2010 Beretta et al.
 7,780,860 B2 8/2010 Higgins et al.
 7,832,566 B2 11/2010 Leach et al.
 7,837,884 B2 11/2010 Dorian et al.
 7,845,499 B2 12/2010 Higgins et al.
 7,901,584 B2 3/2011 Dorian et al.
 7,914,689 B2 3/2011 Higgins et al.
 7,915,029 B2 3/2011 Haubert et al.
 7,919,049 B2 4/2011 Haubert et al.
 7,922,972 B2 4/2011 Ellsworth et al.
 7,954,646 B2 6/2011 Leach et al.
 7,972,578 B2 7/2011 DiCesare et al.
 7,992,725 B2 8/2011 Leach et al.
 8,012,742 B2 9/2011 Haubert et al.
 8,048,320 B2 11/2011 Leach et al.
 8,062,534 B2 11/2011 Higgins et al.
 8,114,680 B2 2/2012 Haubert et al.

RE43,547 E 7/2012 Ellsworth et al.
 8,474,630 B2 7/2013 Dorian et al.
 2002/0023884 A1 2/2002 Anderson
 2002/0094305 A1 7/2002 Dicesare et al.
 2002/0098137 A1 7/2002 Hommeltoft
 2002/0132367 A1 9/2002 Miller et al.
 2002/0156439 A1 10/2002 Iskra
 2003/0205538 A1 11/2003 Dorian et al.
 2004/0013575 A1 1/2004 Stevens et al.
 2004/0043505 A1 3/2004 Walenciak et al.
 2004/0059255 A1 3/2004 Manoussakis et al.
 2004/0129631 A1 7/2004 Anraku et al.
 2004/0166029 A1 8/2004 Losada et al.
 2004/0210196 A1 10/2004 Bush Jr et al.
 2004/0241364 A1 12/2004 Zihlmann
 2004/0256331 A1 12/2004 Arking et al.
 2005/0059163 A1 3/2005 Dastane et al.
 2005/0124965 A1 6/2005 Haywood
 2005/0186120 A1 8/2005 Dorian et al.
 2005/0261620 A1 11/2005 Ballin
 2006/0032825 A1 2/2006 Ellsworth et al.
 2006/0212020 A1 9/2006 Rainen et al.
 2006/0263266 A1 11/2006 DiCesare et al.
 2006/0278588 A1 12/2006 Woodell-May
 2007/0020629 A1 1/2007 Ross et al.
 2007/0034579 A1 2/2007 Dorian et al.
 2011/0151256 A1* 6/2011 Wang et al. 428/373
 2012/0015796 A1 1/2012 Leach et al.
 2012/0279973 A1* 11/2012 Capitani 220/669

FOREIGN PATENT DOCUMENTS

EP 0119692 B1 9/1984
 EP 0137292 B1 3/1990
 EP 0392377 A2 10/1990
 EP 0184274 B1 5/1992
 EP 0385953 B1 4/1993
 EP 0537507 A1 4/1993
 EP 0399151 B1 8/1994
 EP 0520184 B1 1/1996
 EP 0520185 B1 2/1996
 EP 0753741 A1 1/1997
 EP 0494079 B1 3/1997
 EP 0766973 A1 4/1997
 EP 0493838 B1 5/1997
 EP 0627261 B1 5/1998
 EP 0640215 B1 11/1998
 EP 0817680 B1 12/1999
 EP 0678557 B1 6/2000
 EP 1016460 A2 7/2000
 EP 0688606 B1 12/2000
 EP 1106253 A2 6/2001
 EP 0739229 B1 10/2001
 EP 1205250 A1 5/2002
 EP 0875757 B1 6/2003
 GB 2293986 A 4/1996
 JP 49047973 A 5/1974
 JP 55055259 A 4/1980
 JP 56118669 A 9/1981
 JP 59020856 A 2/1984
 JP 3270701 A 12/1991
 JP 581712 U 11/1993
 JP 9292393 A 11/1997
 JP 11314011 11/1999
 JP 2000189407 7/2000
 JP 2000199760 7/2000
 JP 2003185653 A 7/2003
 WO 9520675 A1 8/1995
 WO 9605770 A1 2/1996
 WO 9607097 A1 3/1996
 WO 9609308 A1 3/1996
 WO 9851411 A2 11/1998
 WO 0114850 A1 3/2001
 WO 02073190 A1 9/2002
 WO 03035888 A1 5/2003

* cited by examiner

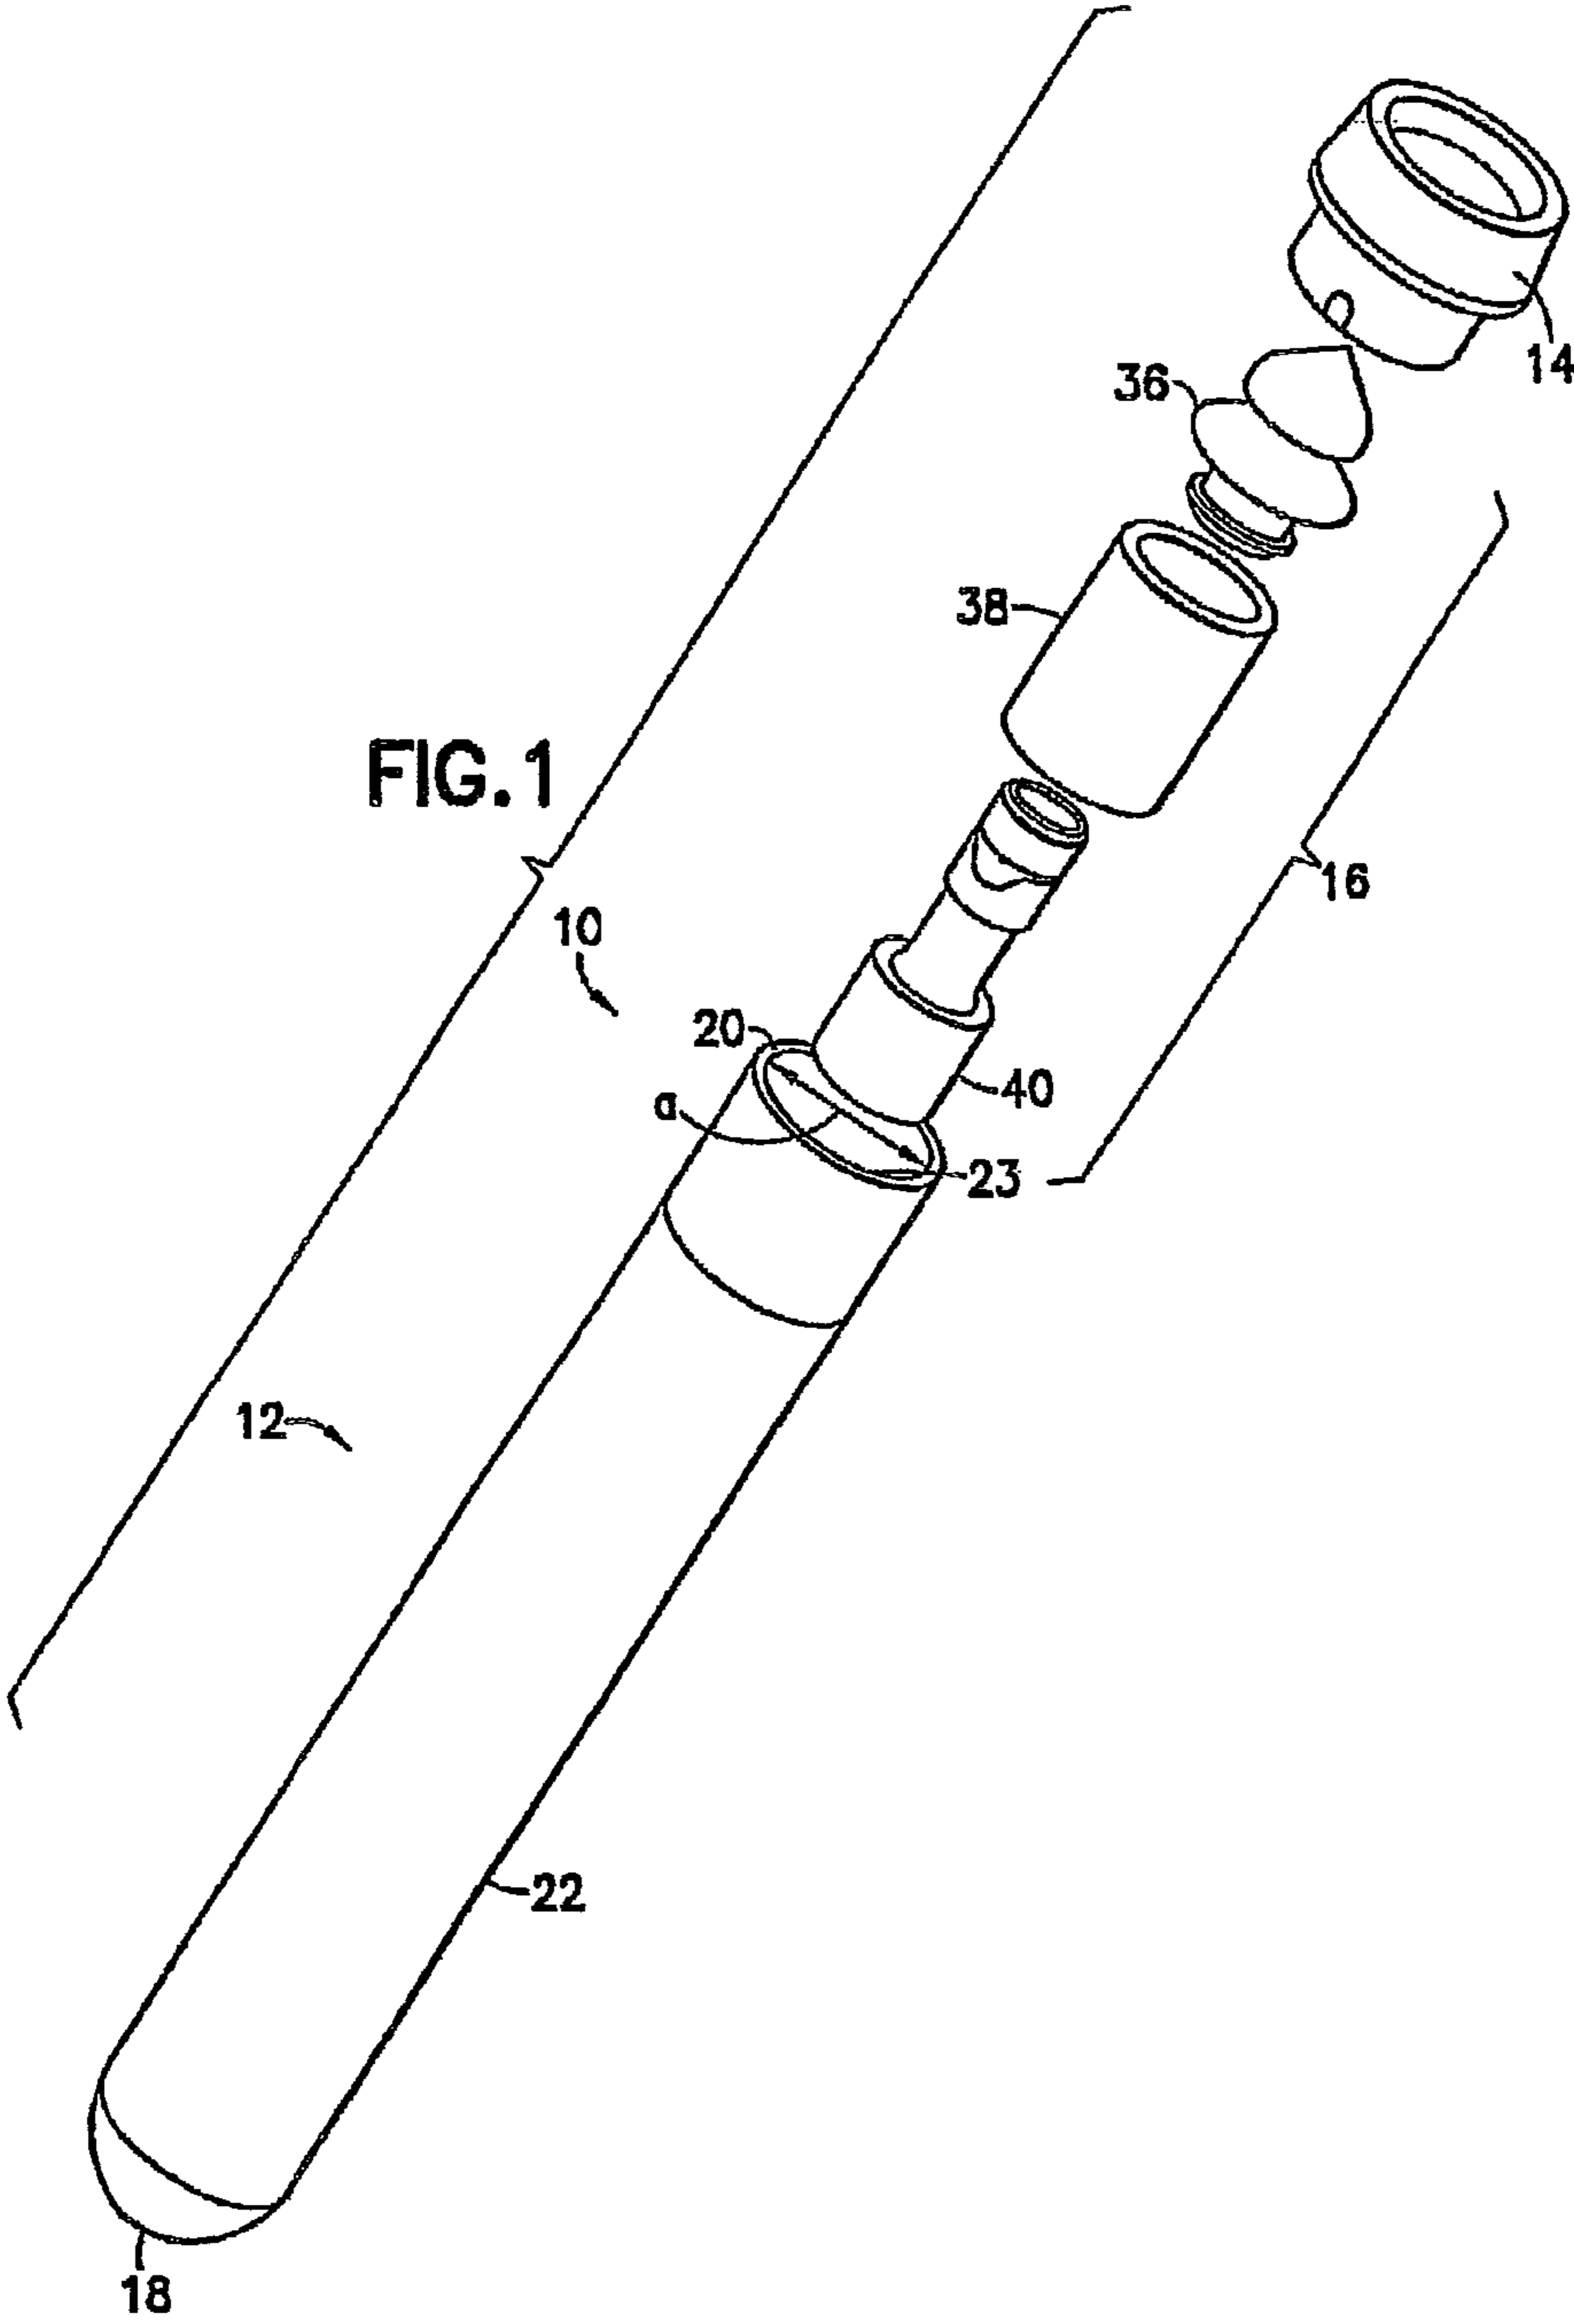

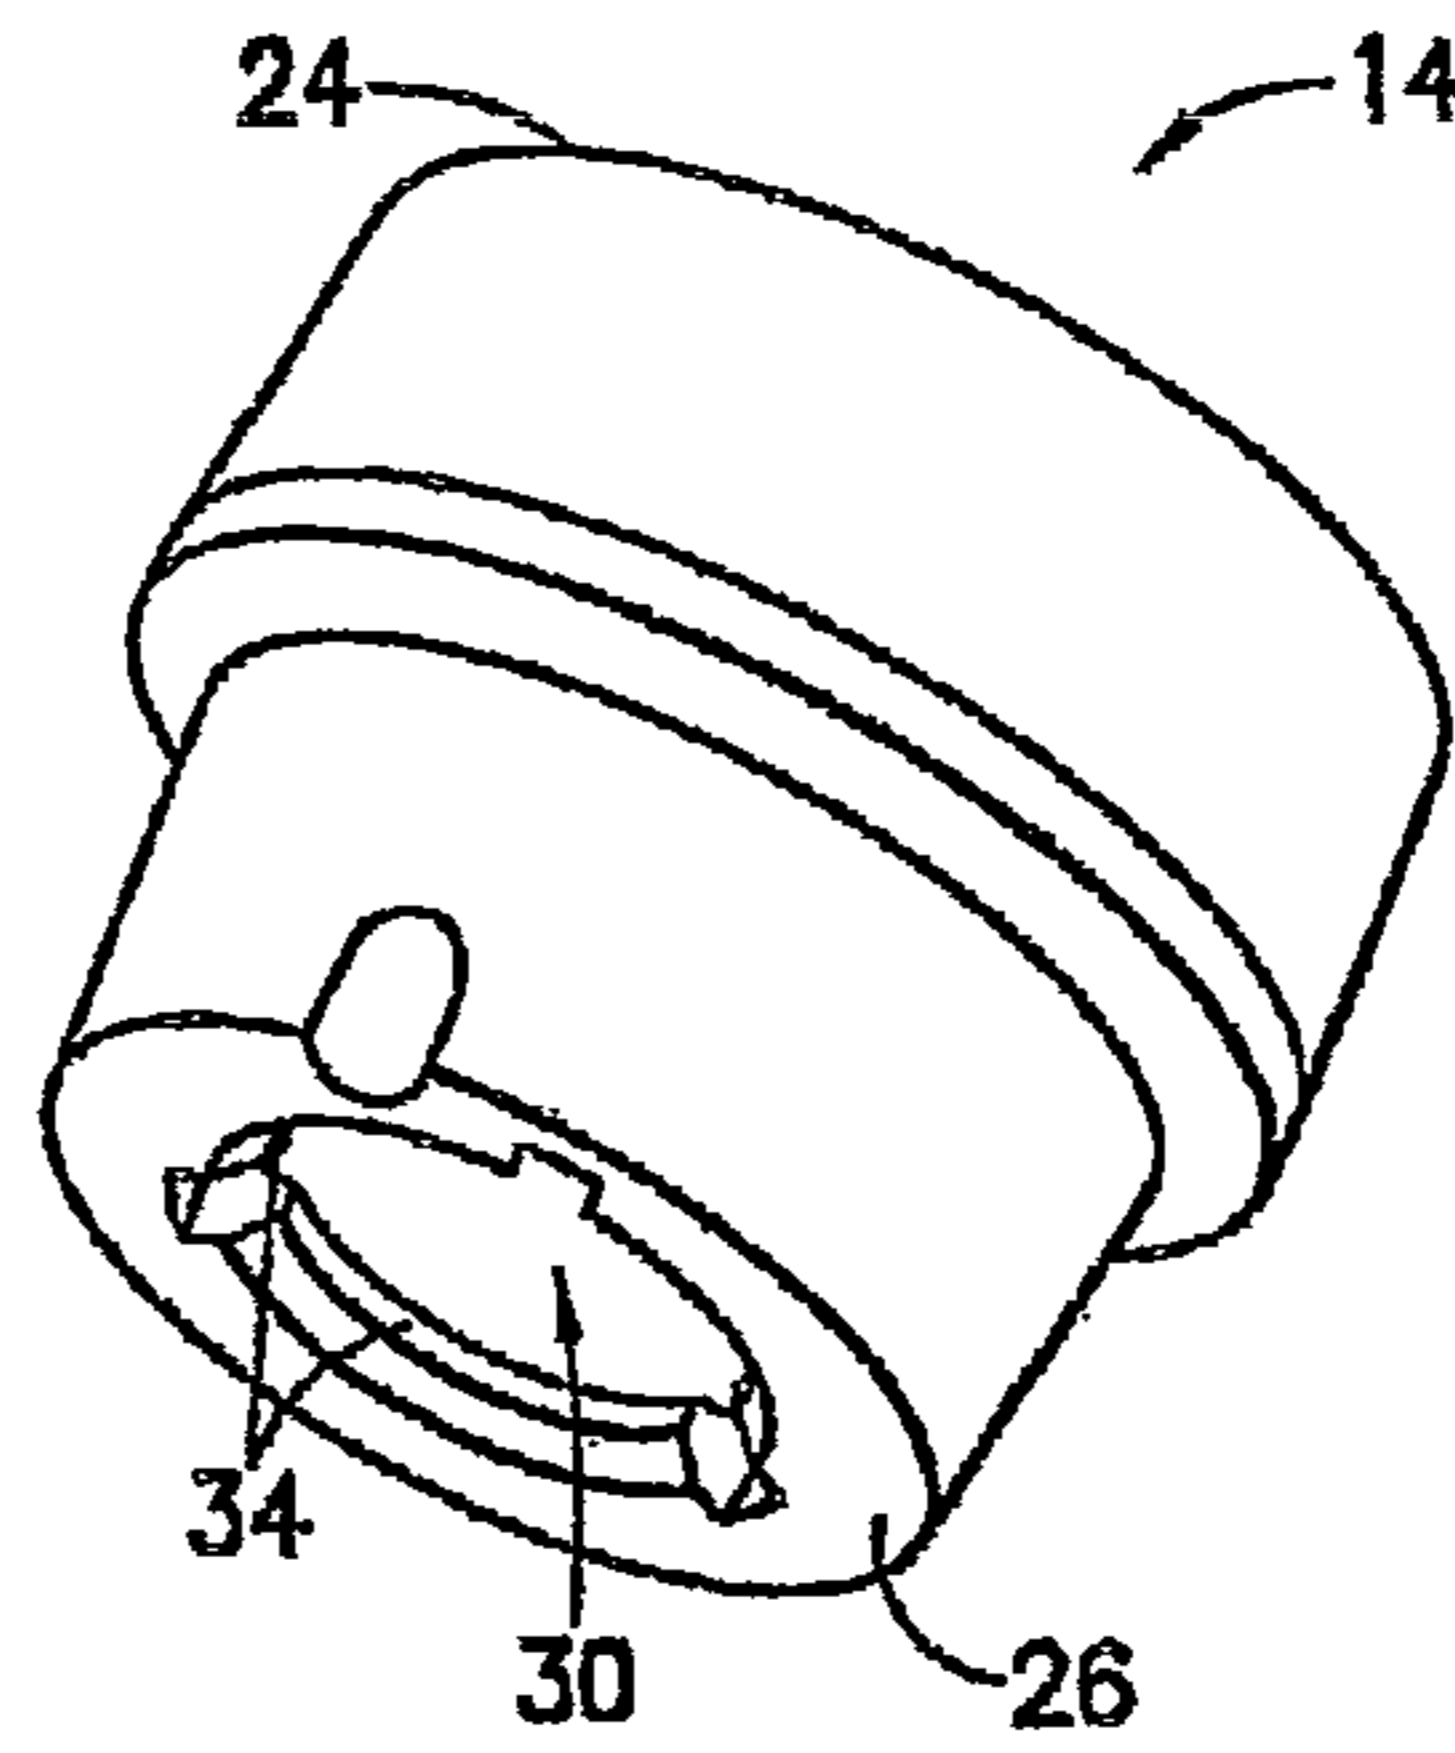


FIG. 2

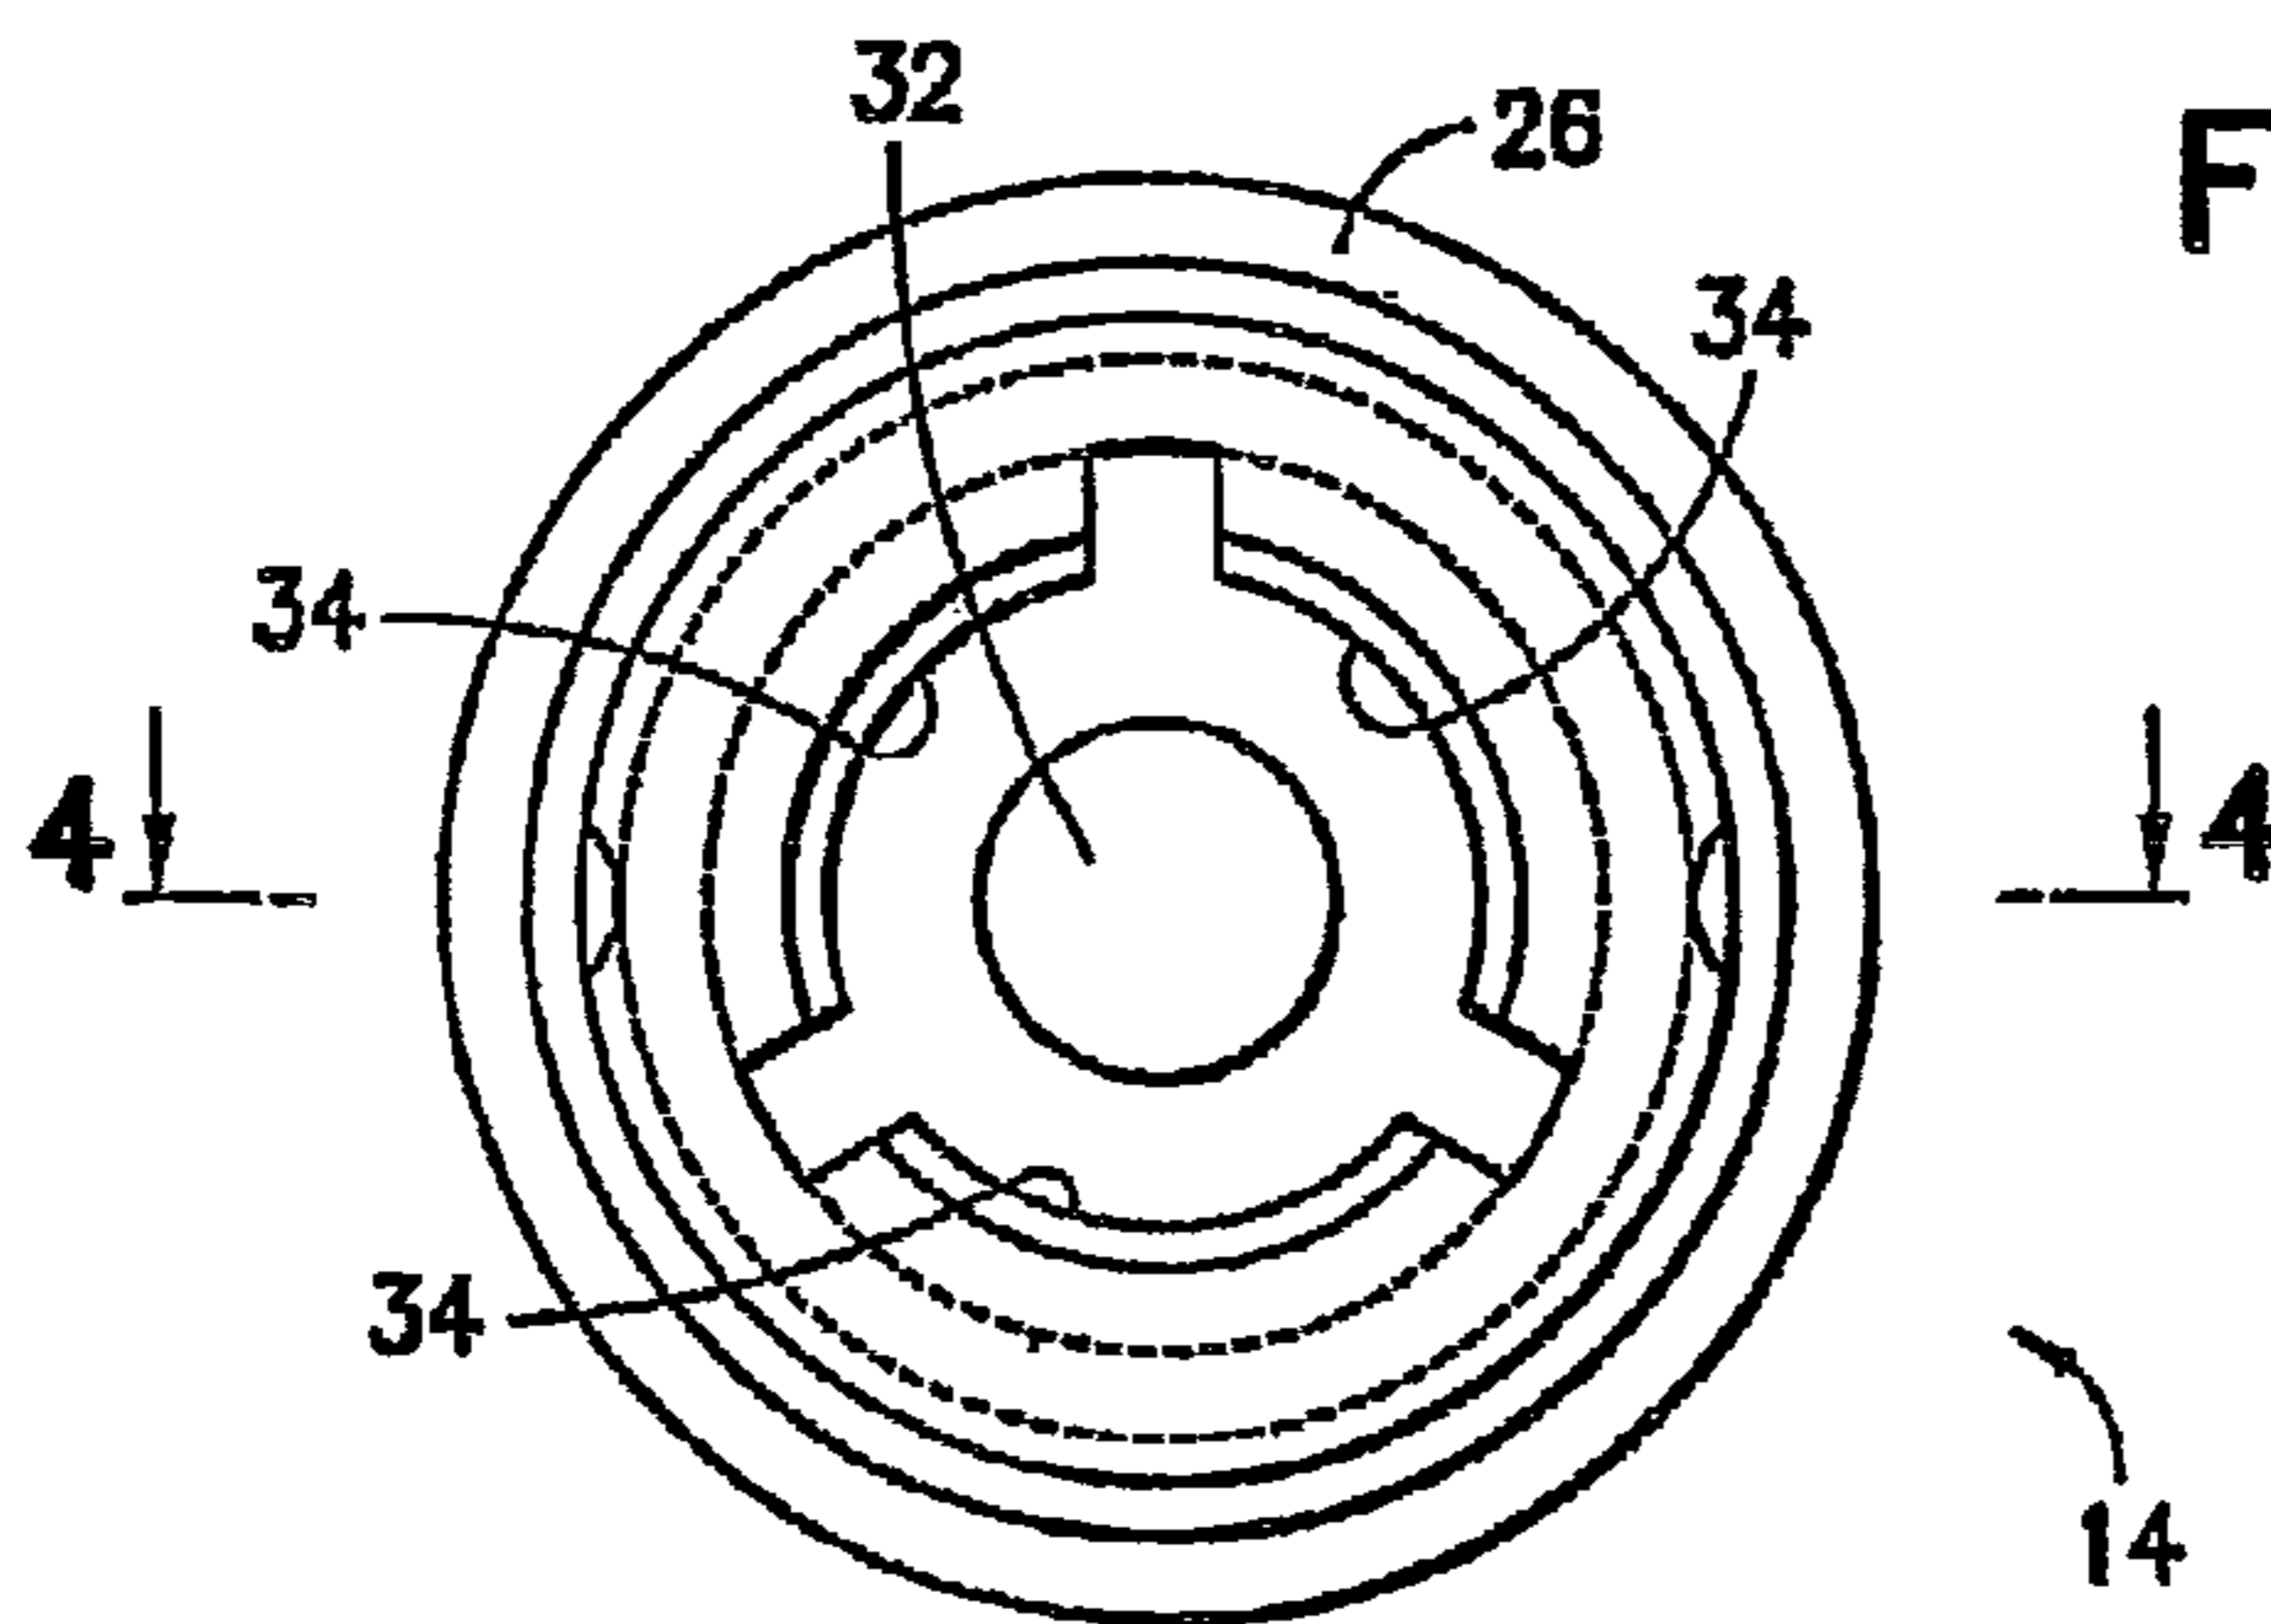


FIG. 3

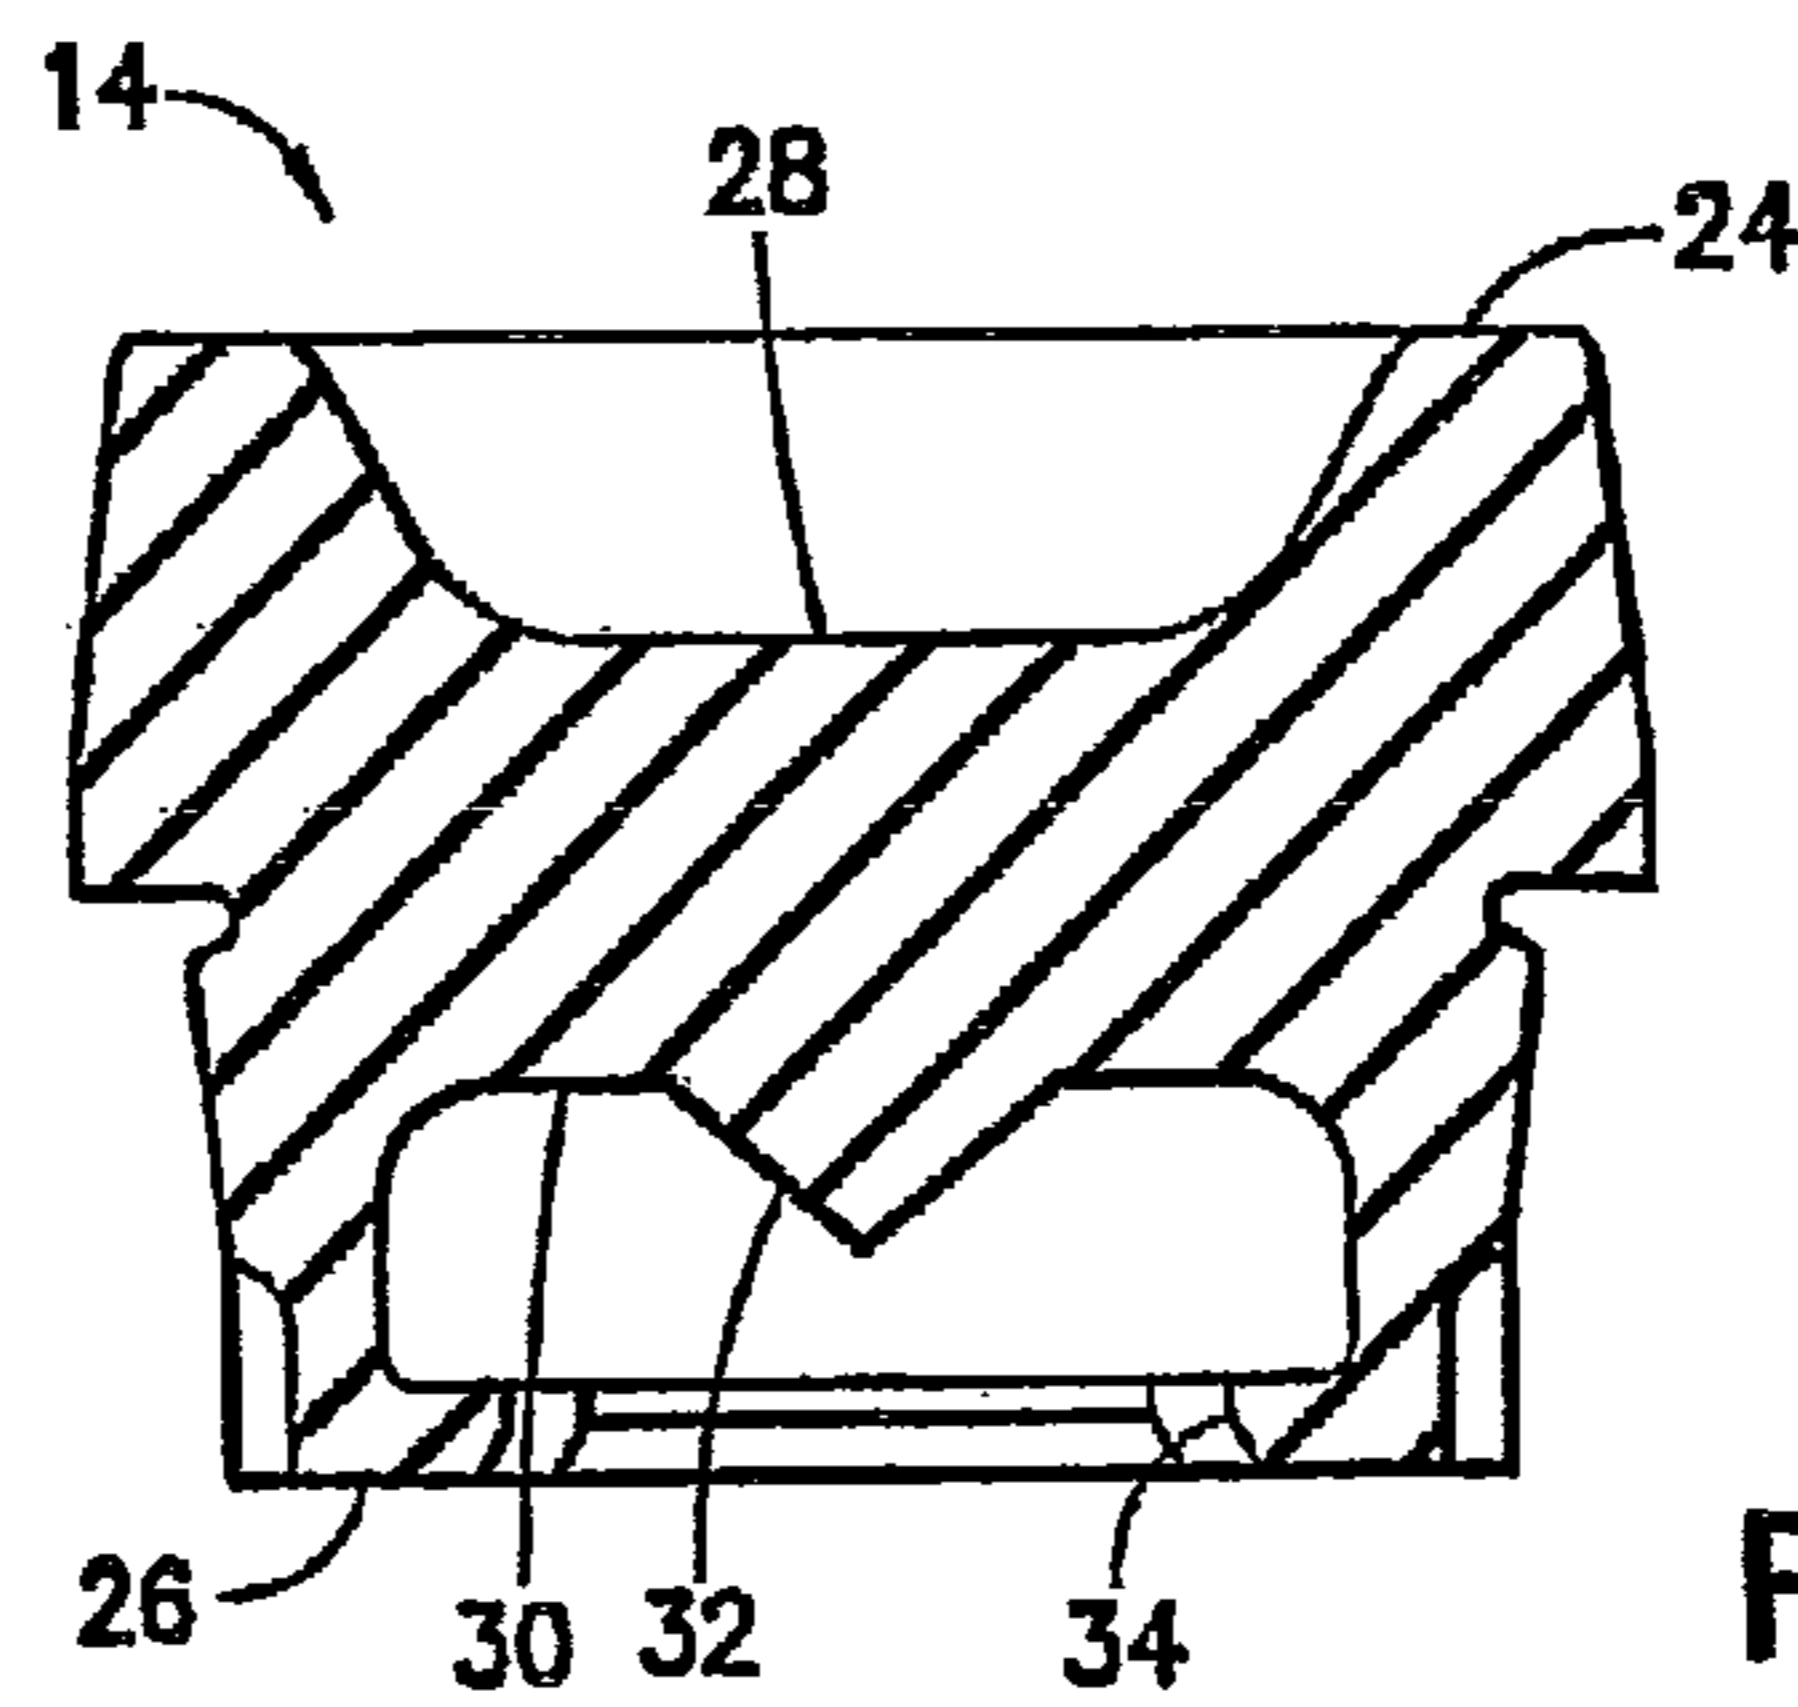


FIG. 4

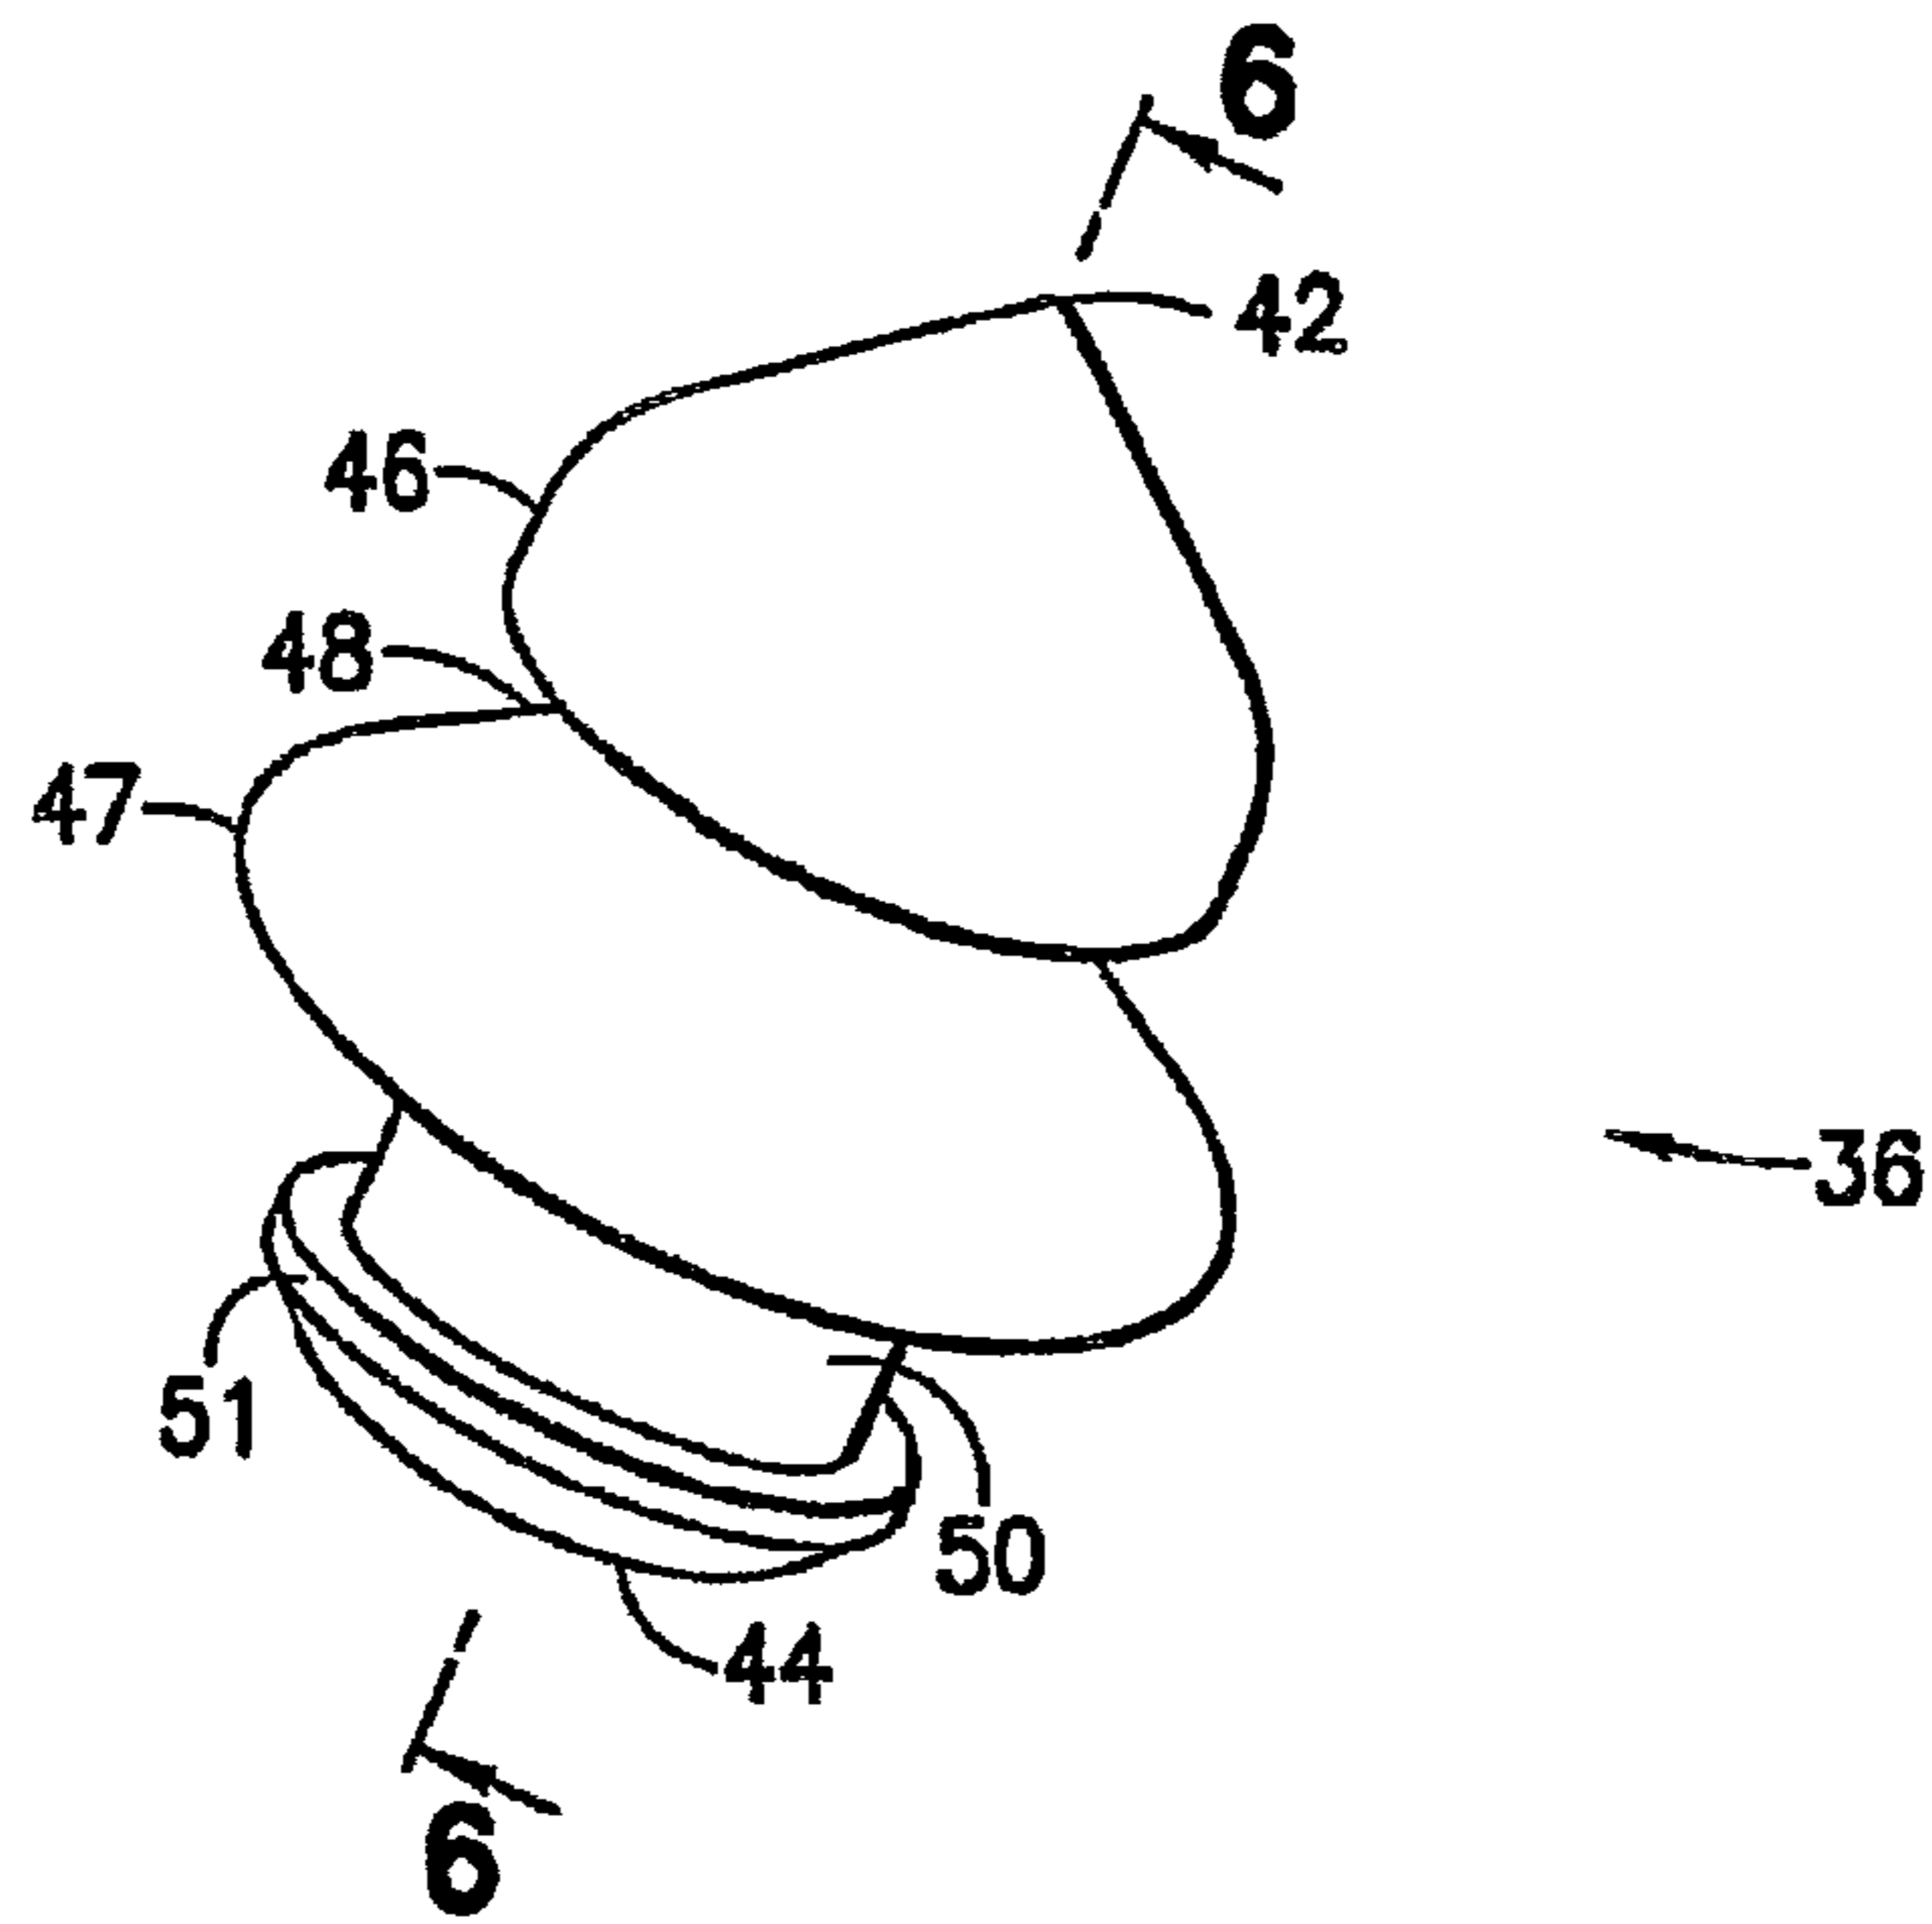


FIG. 5

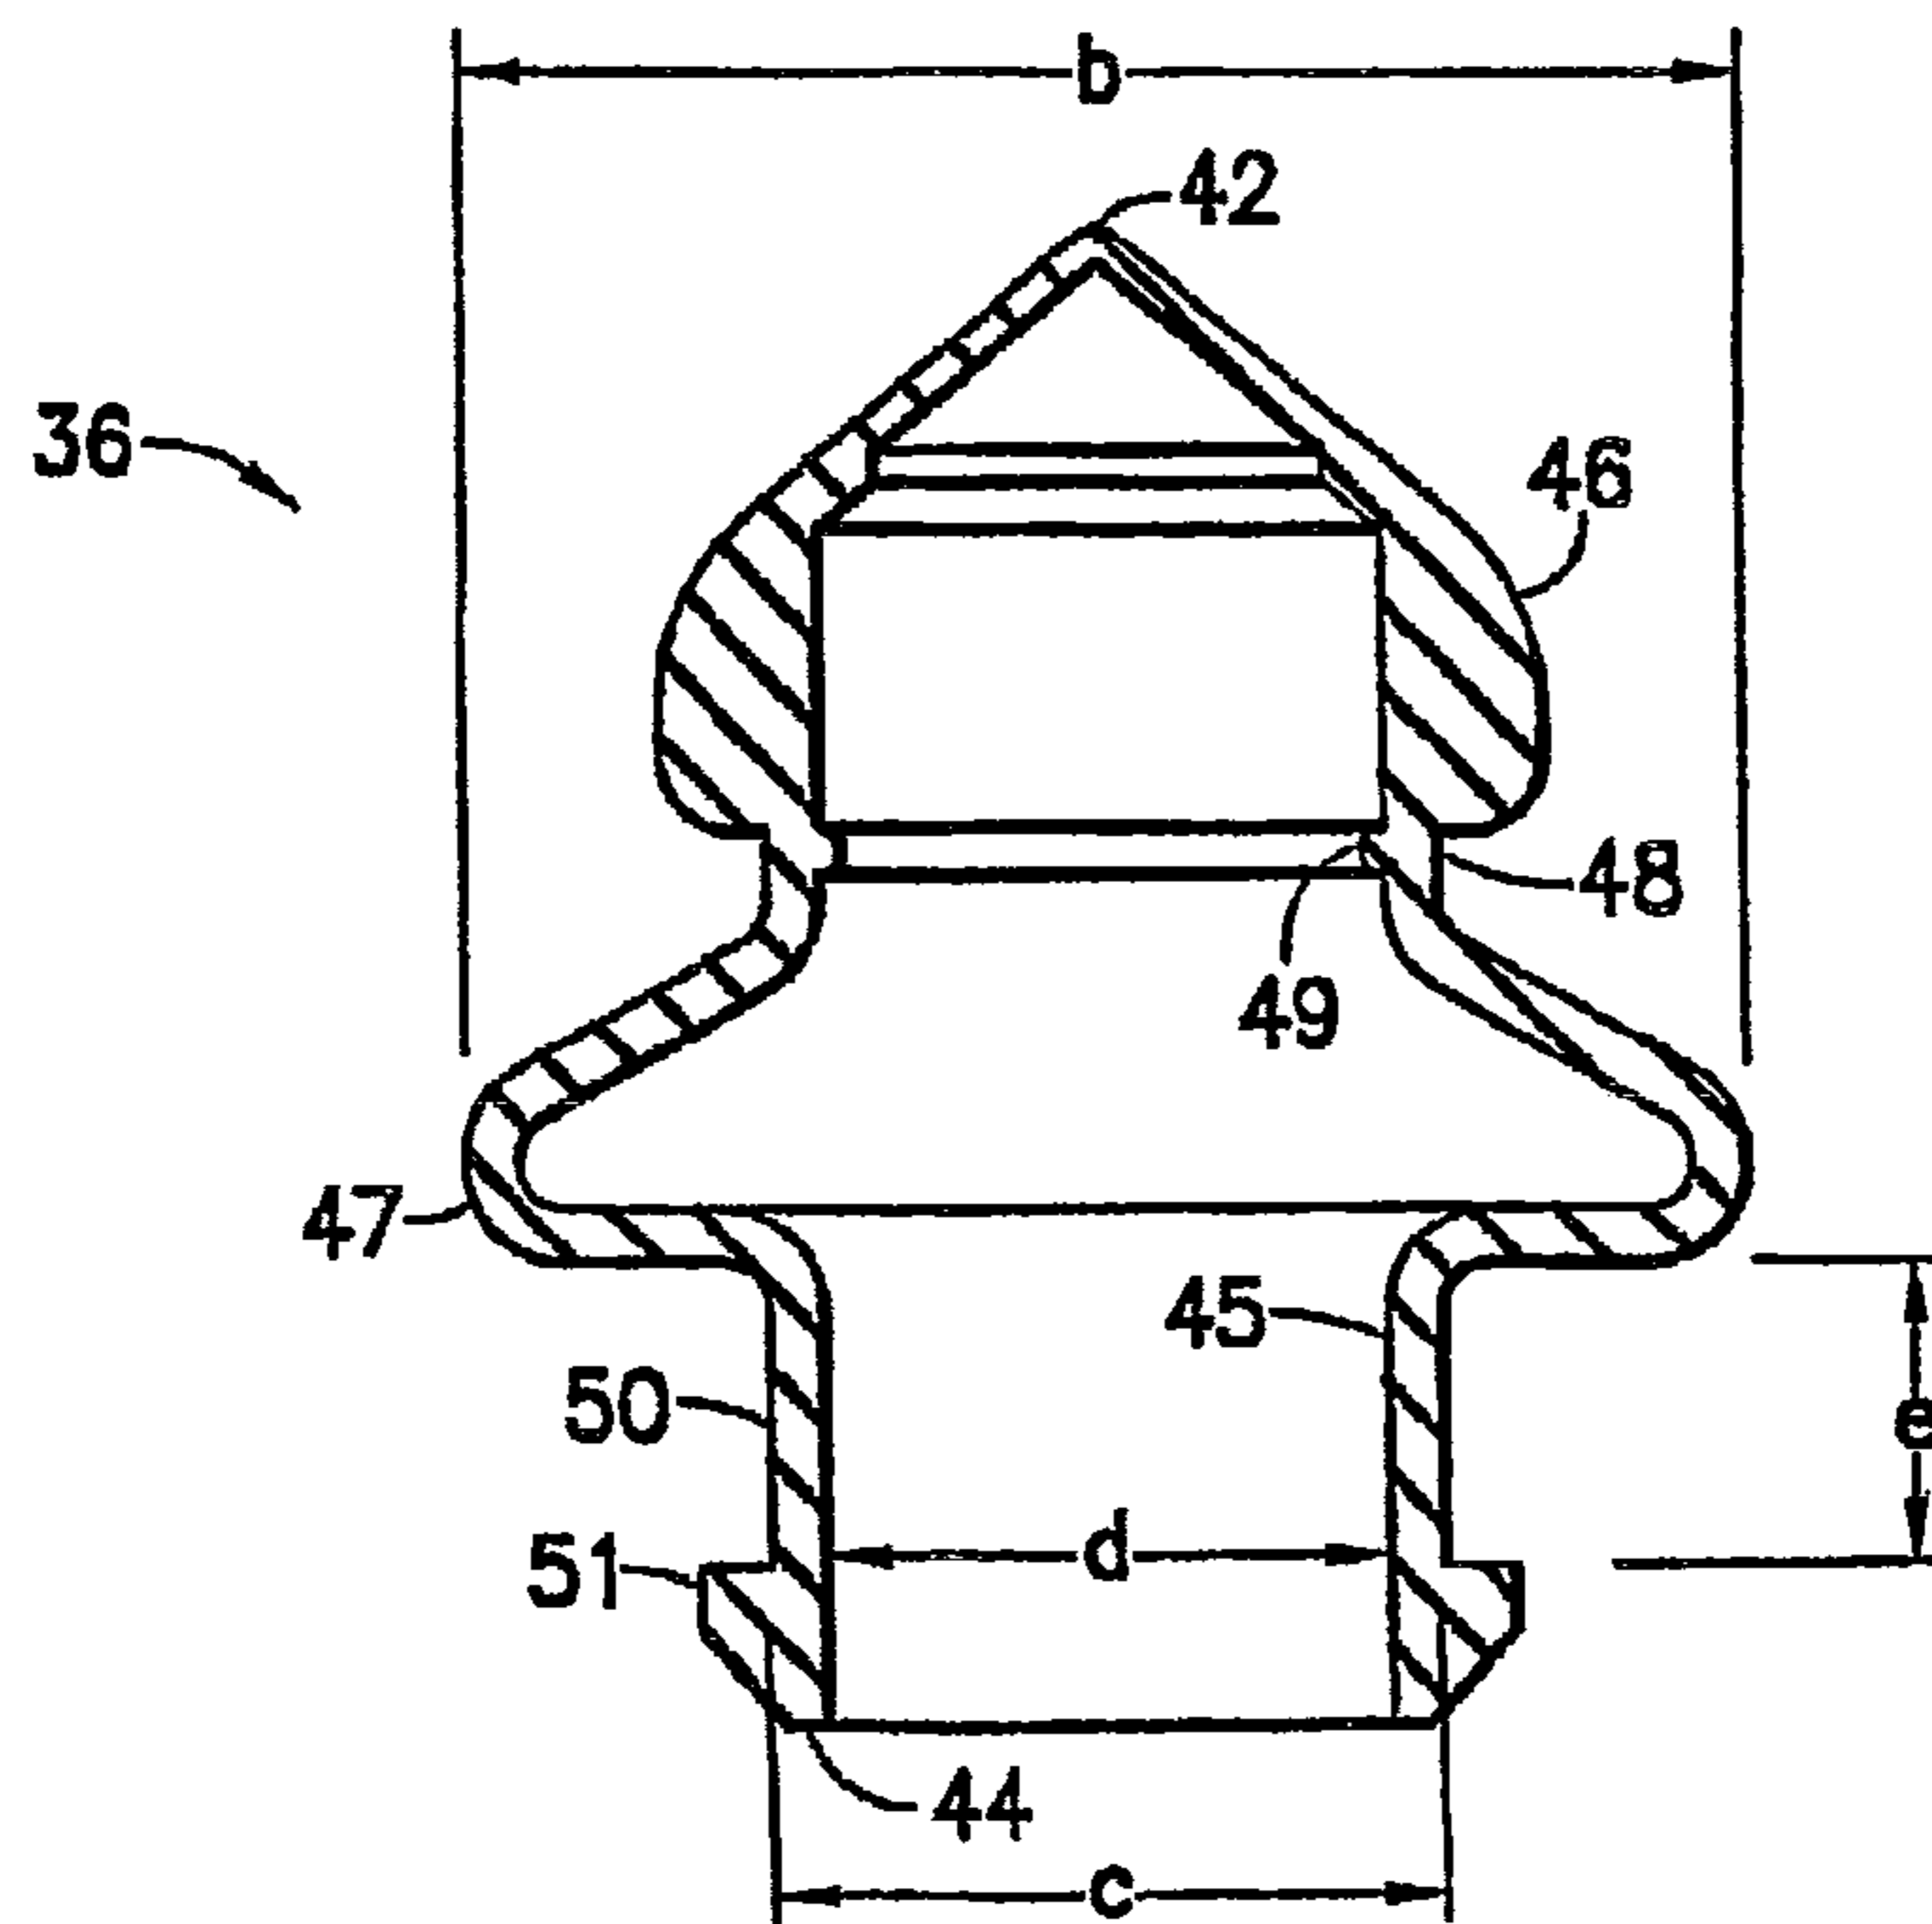


FIG. 6

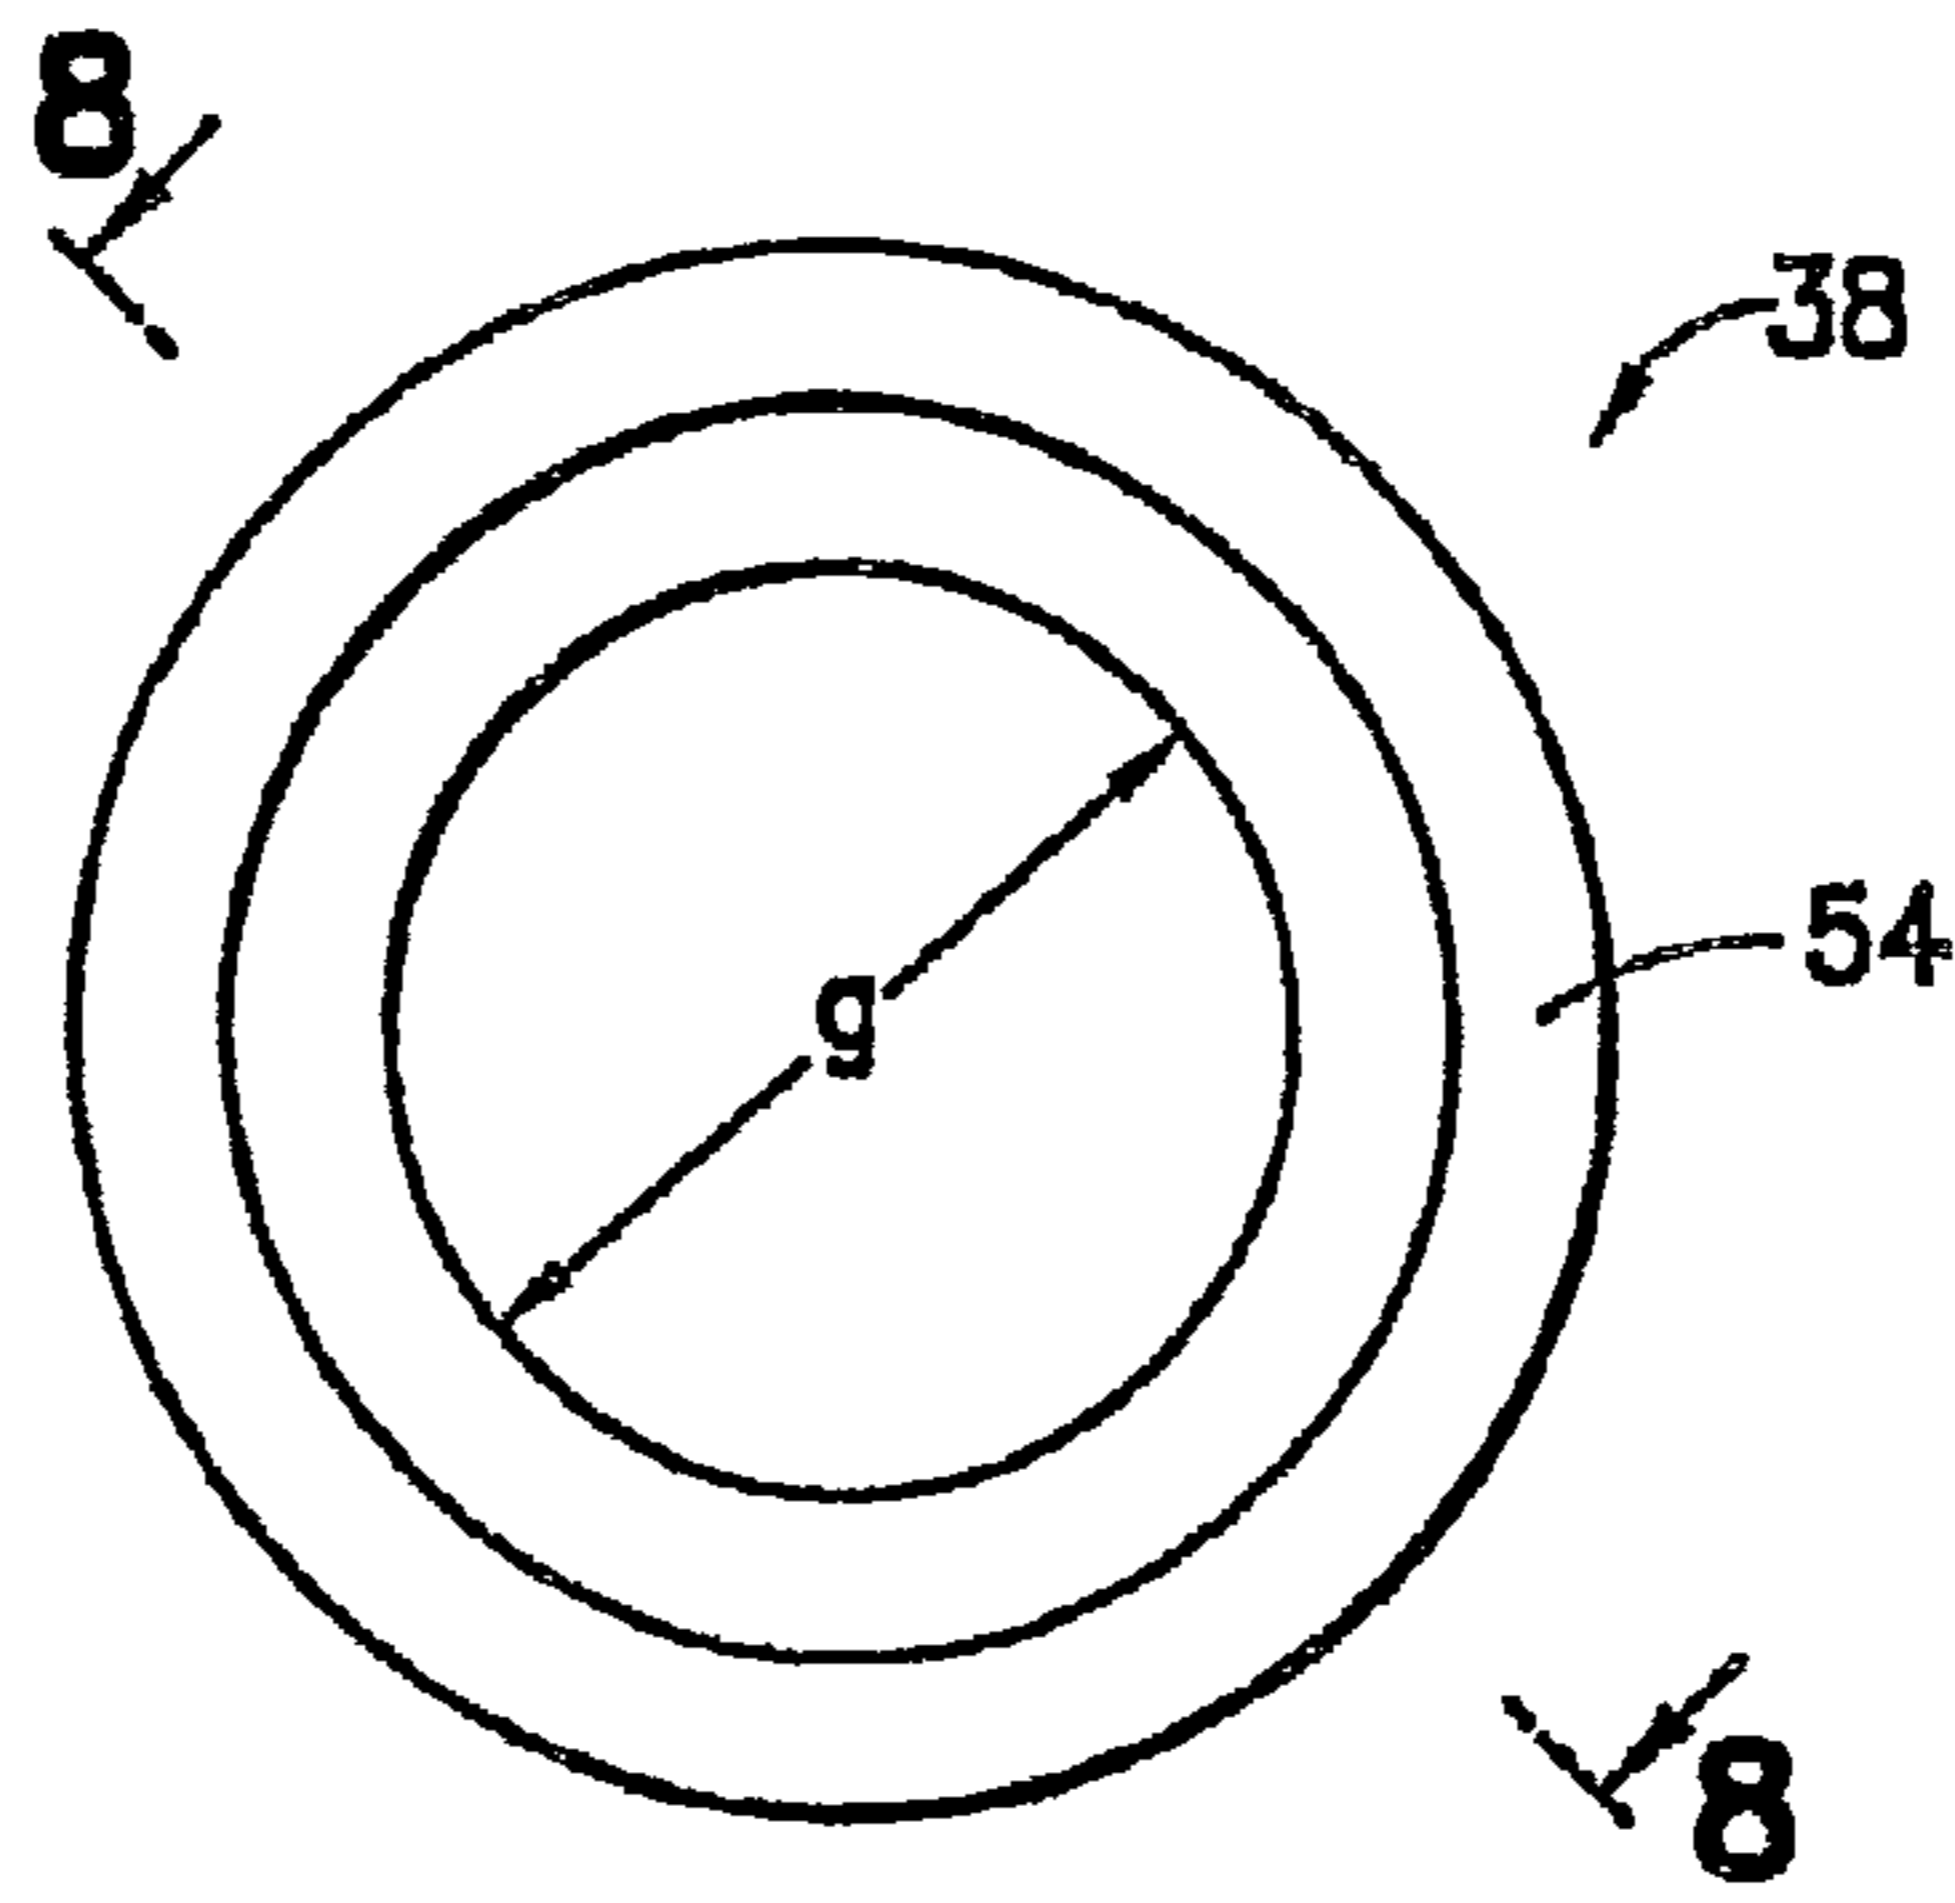


FIG. 7

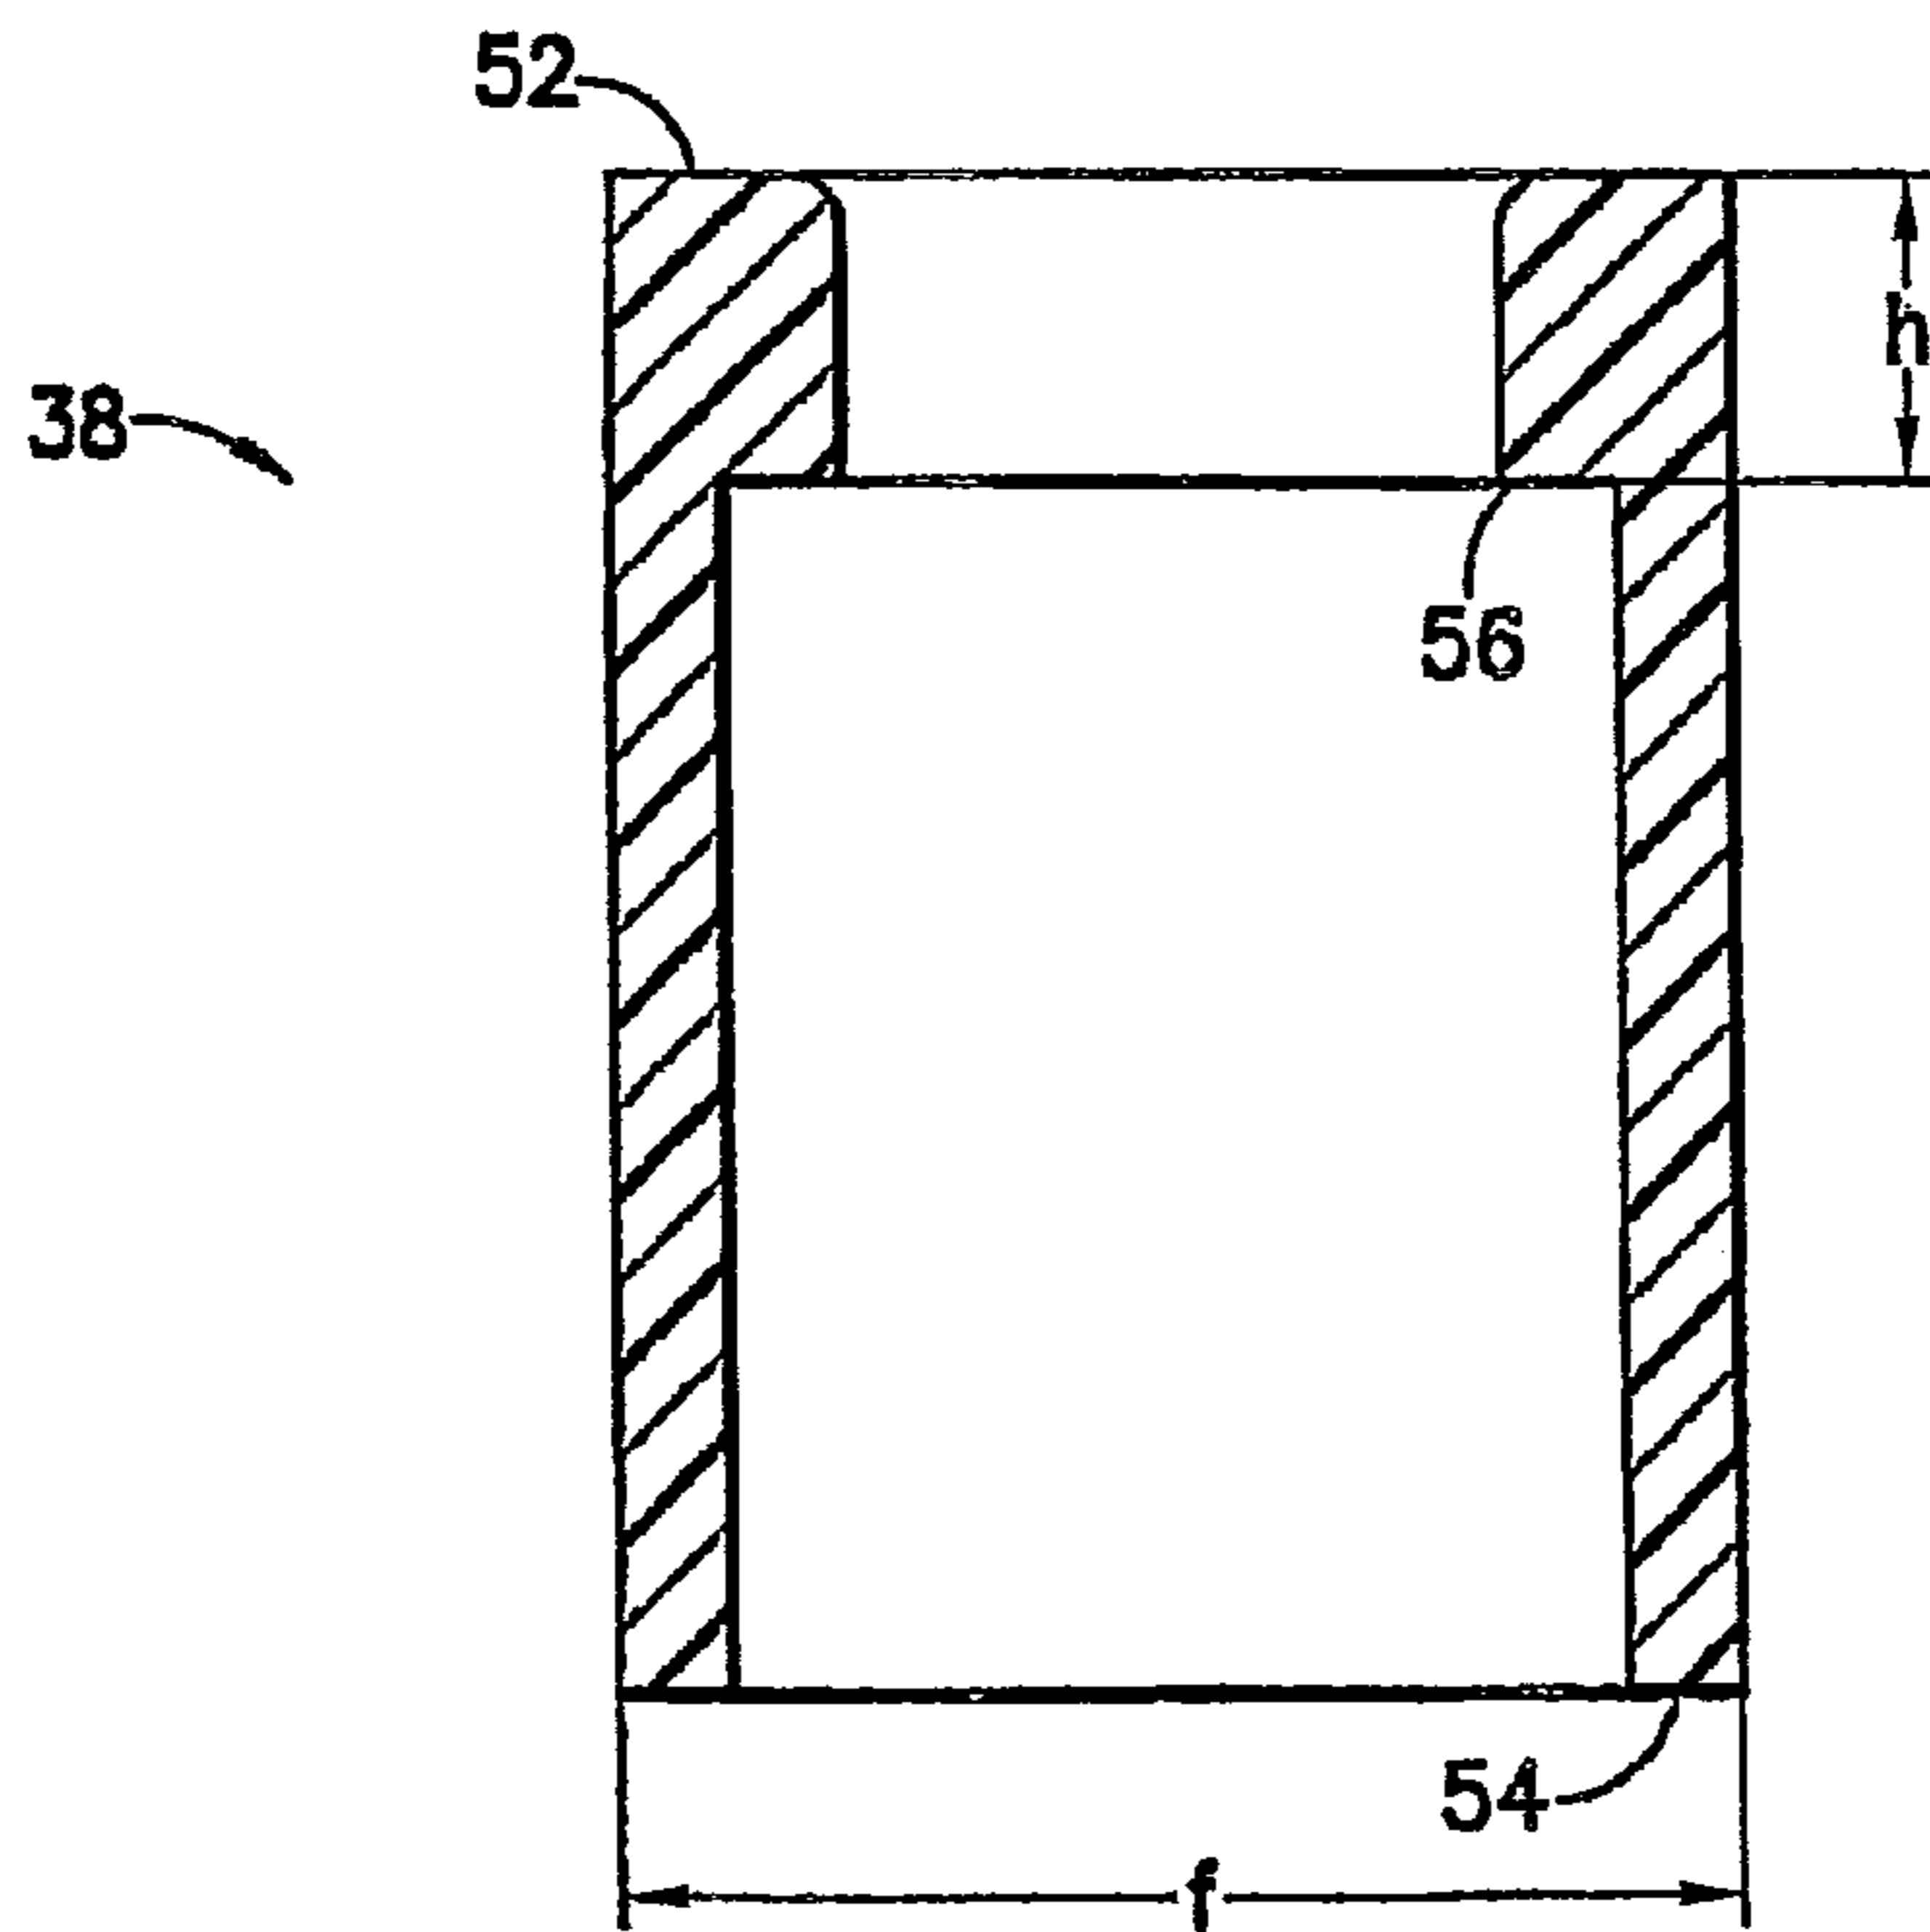


FIG. 8

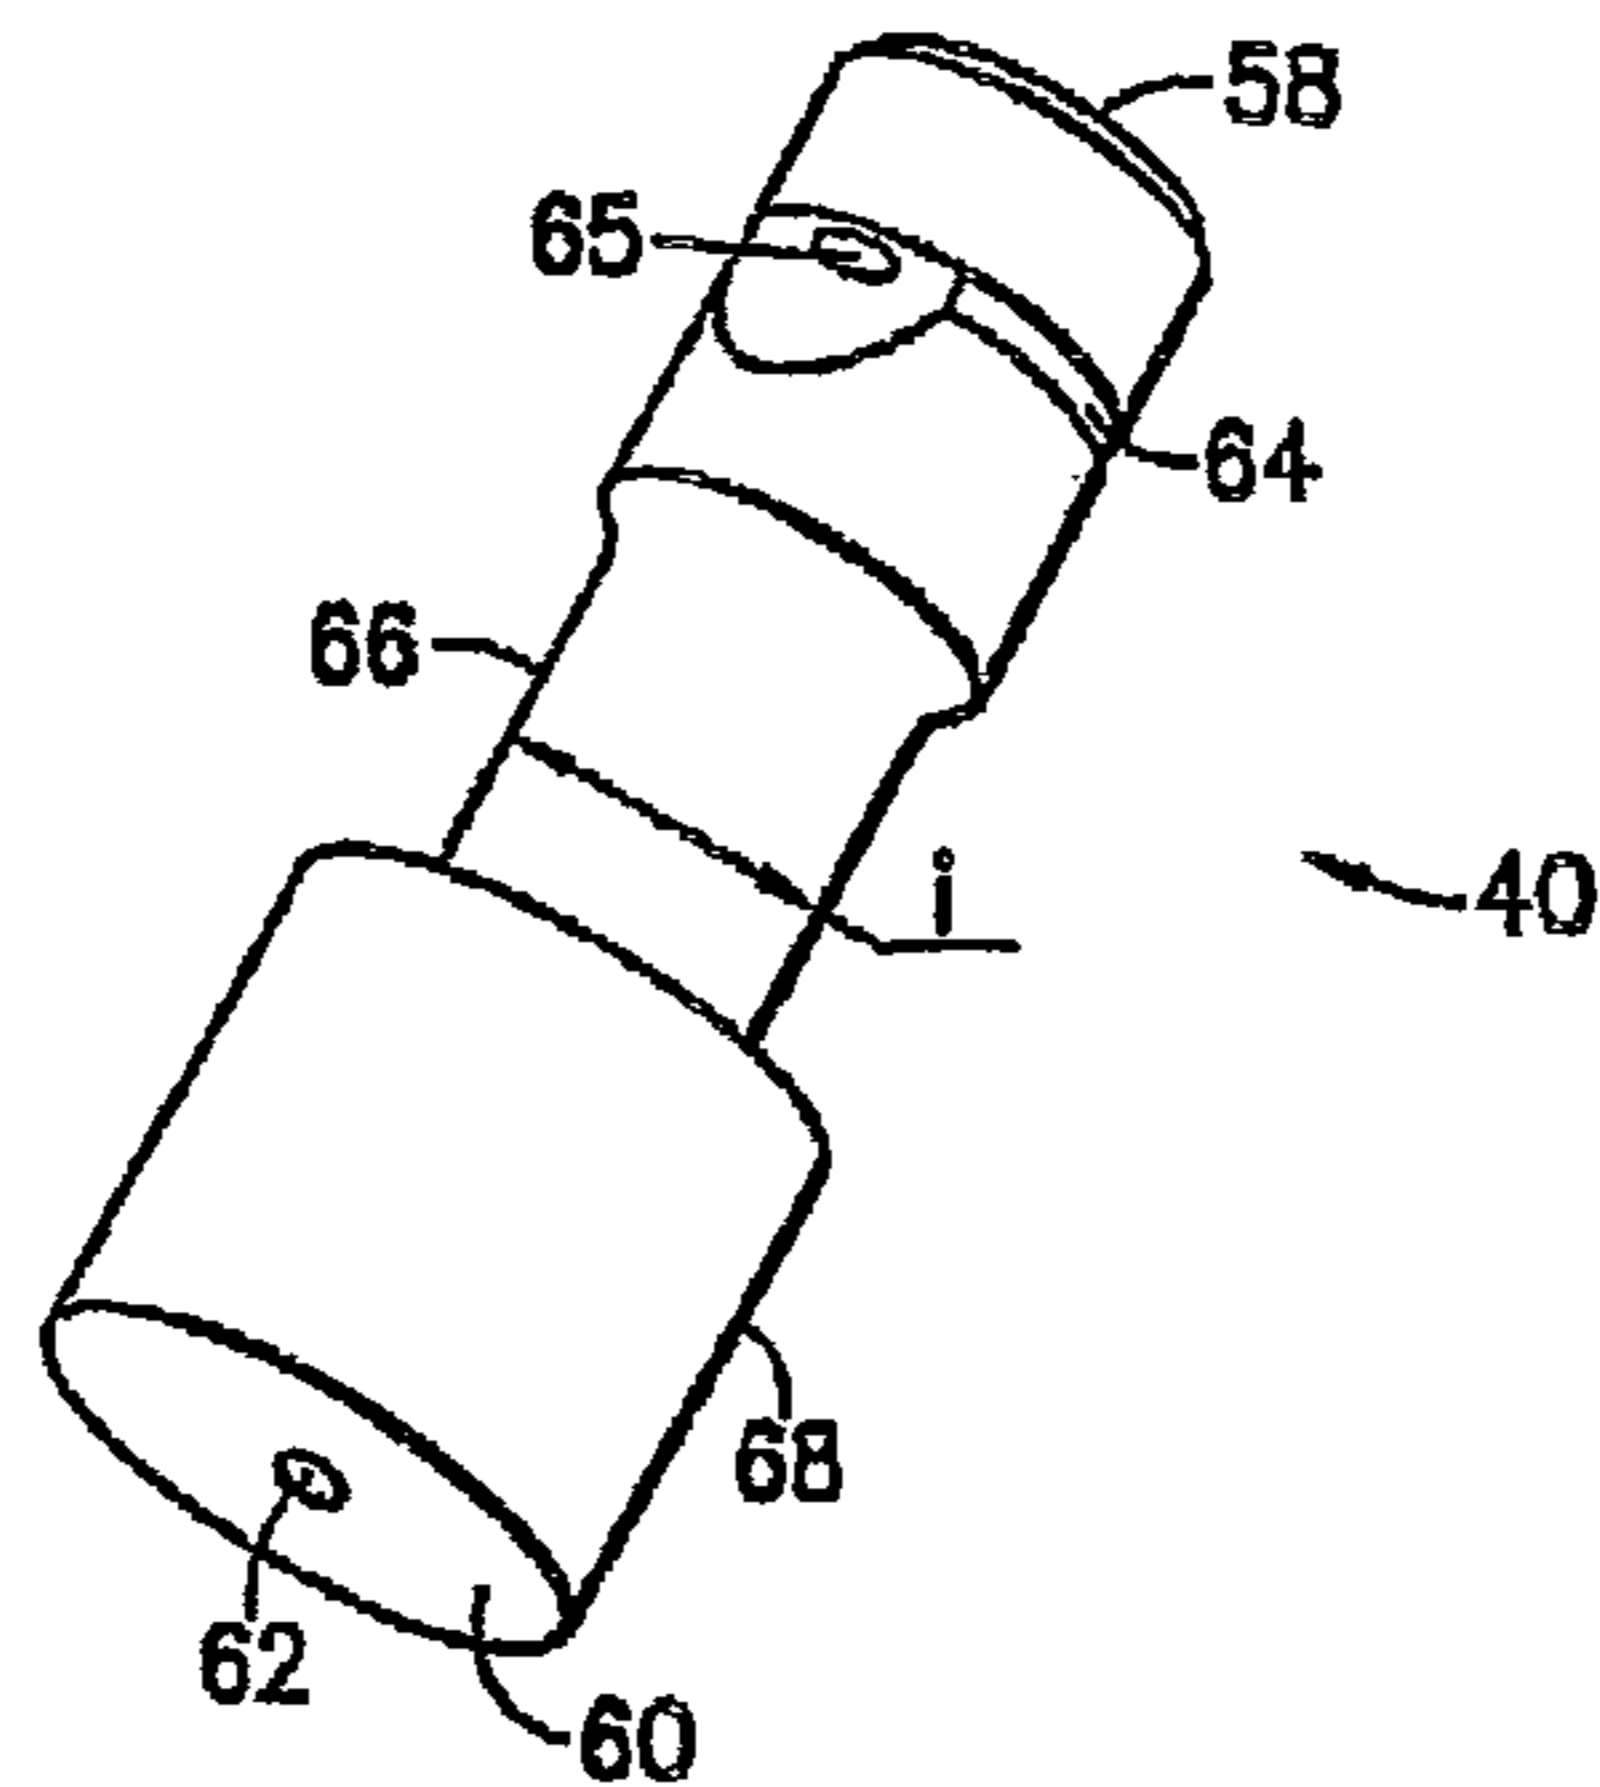


FIG. 9

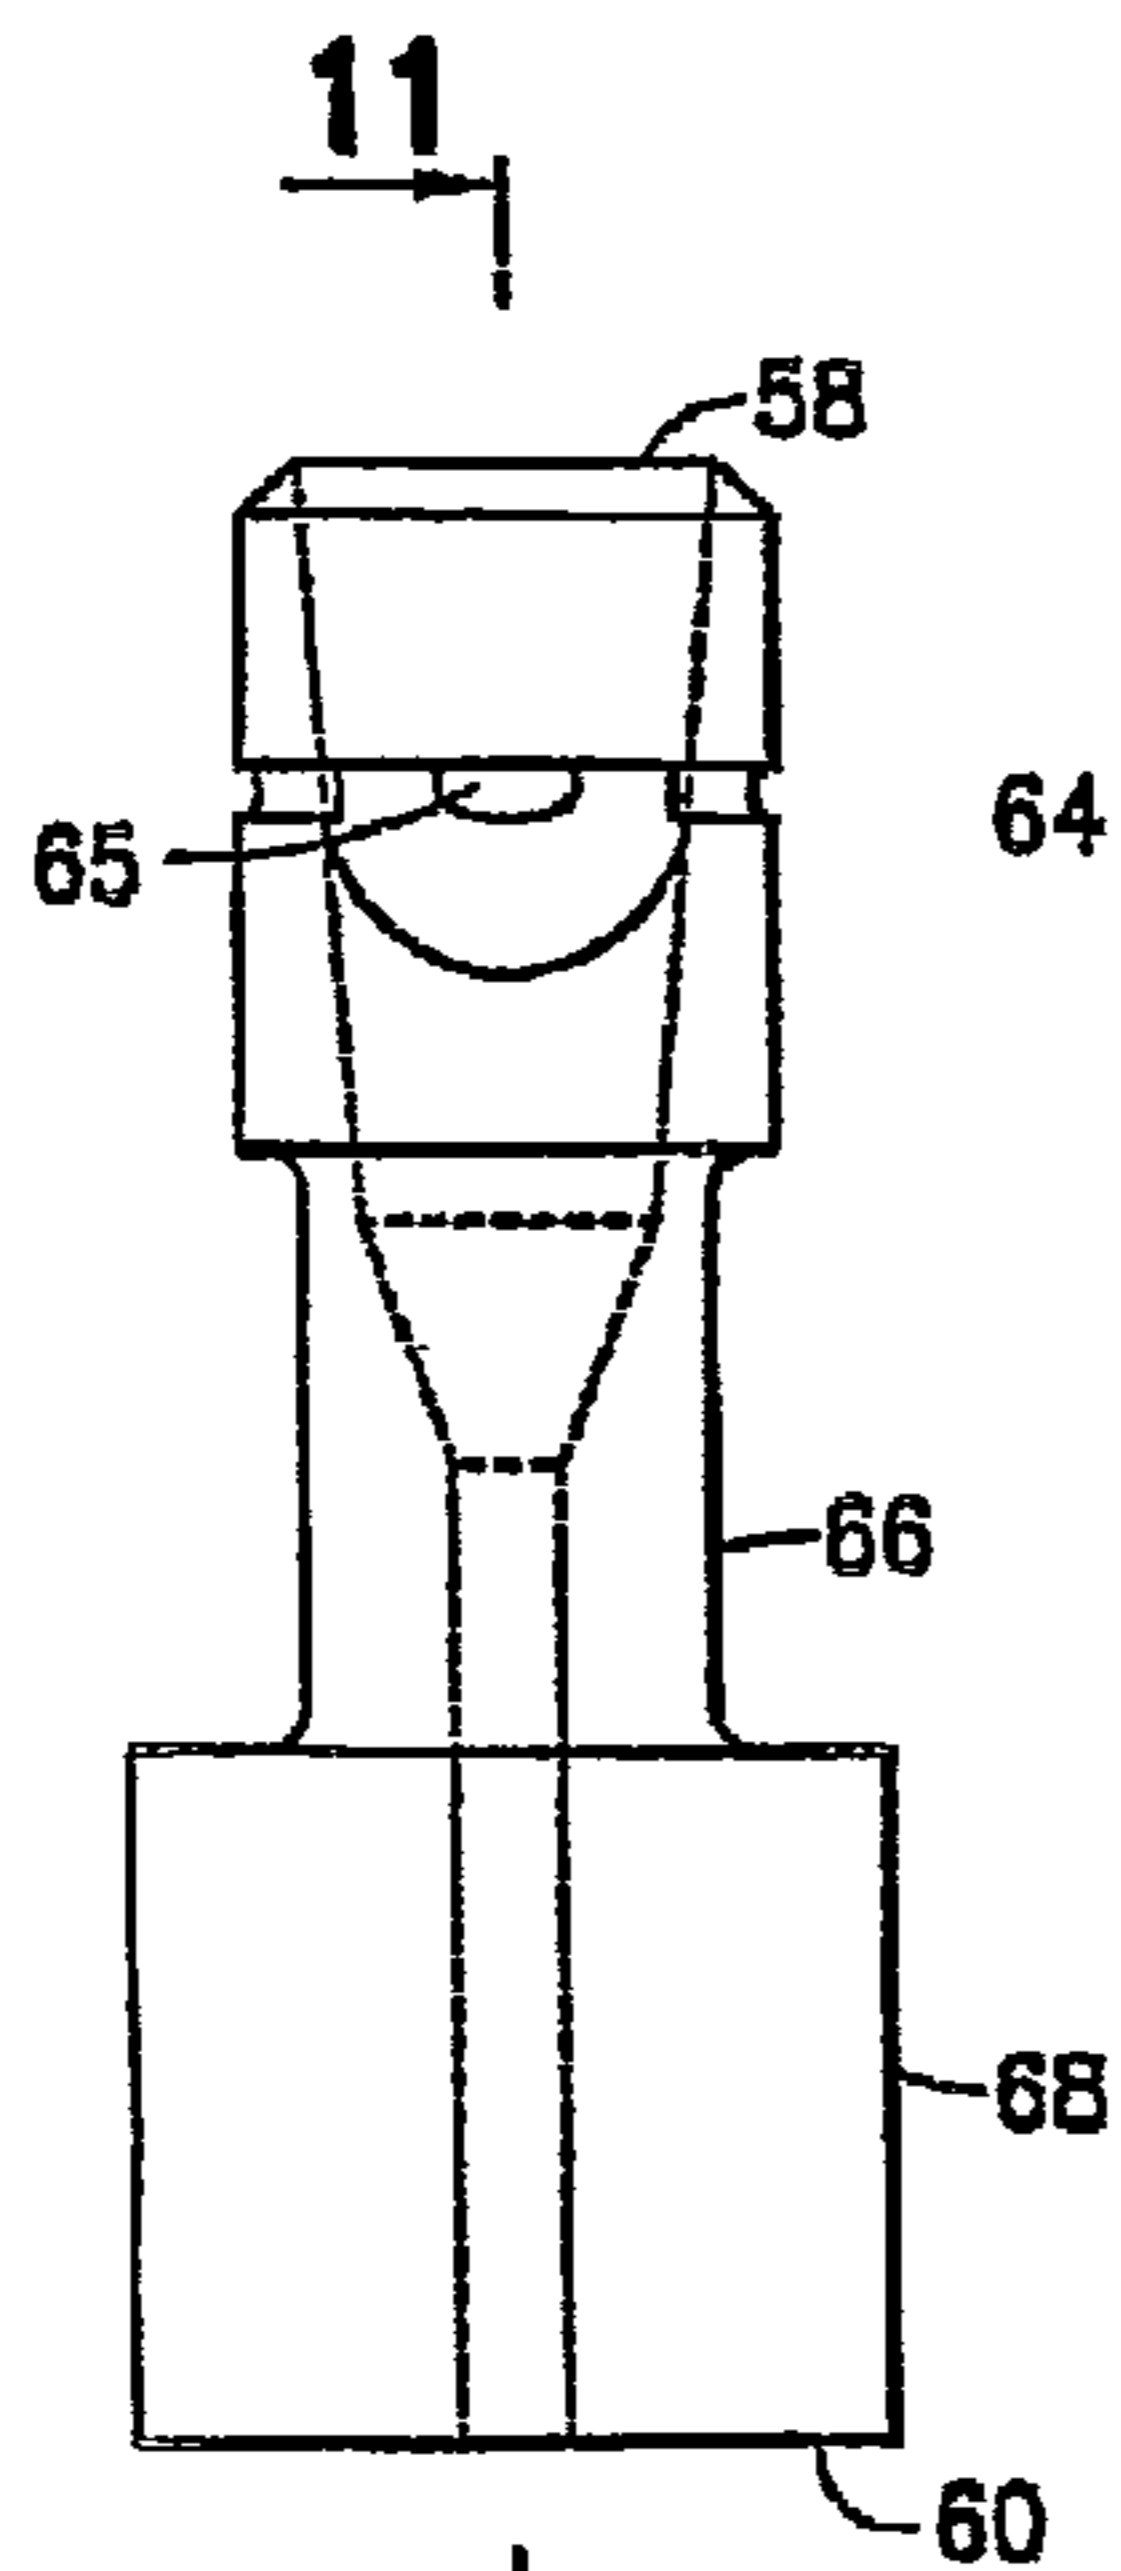


FIG. 10

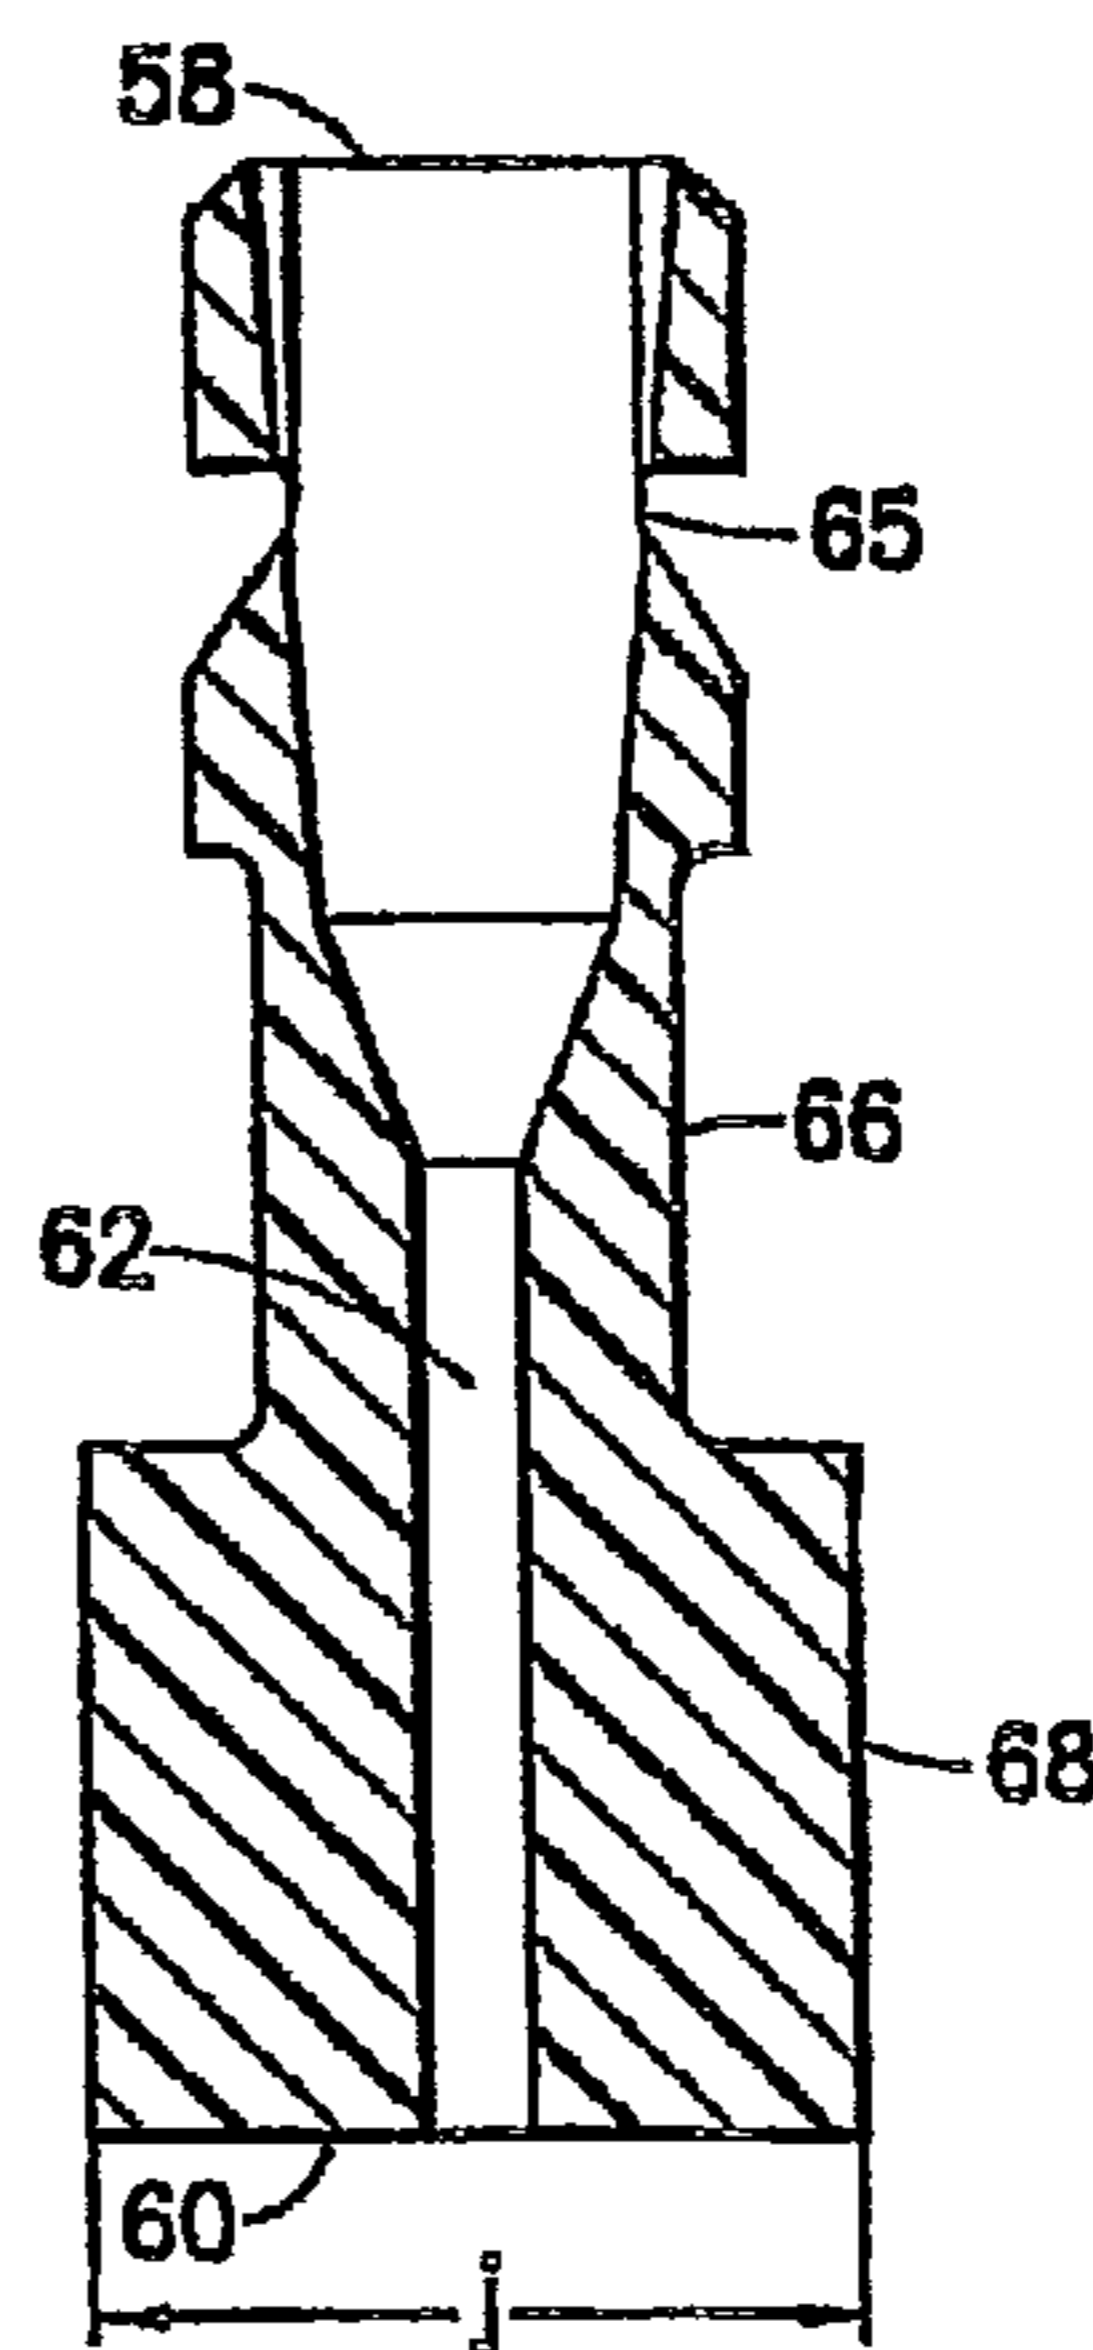


FIG. 11

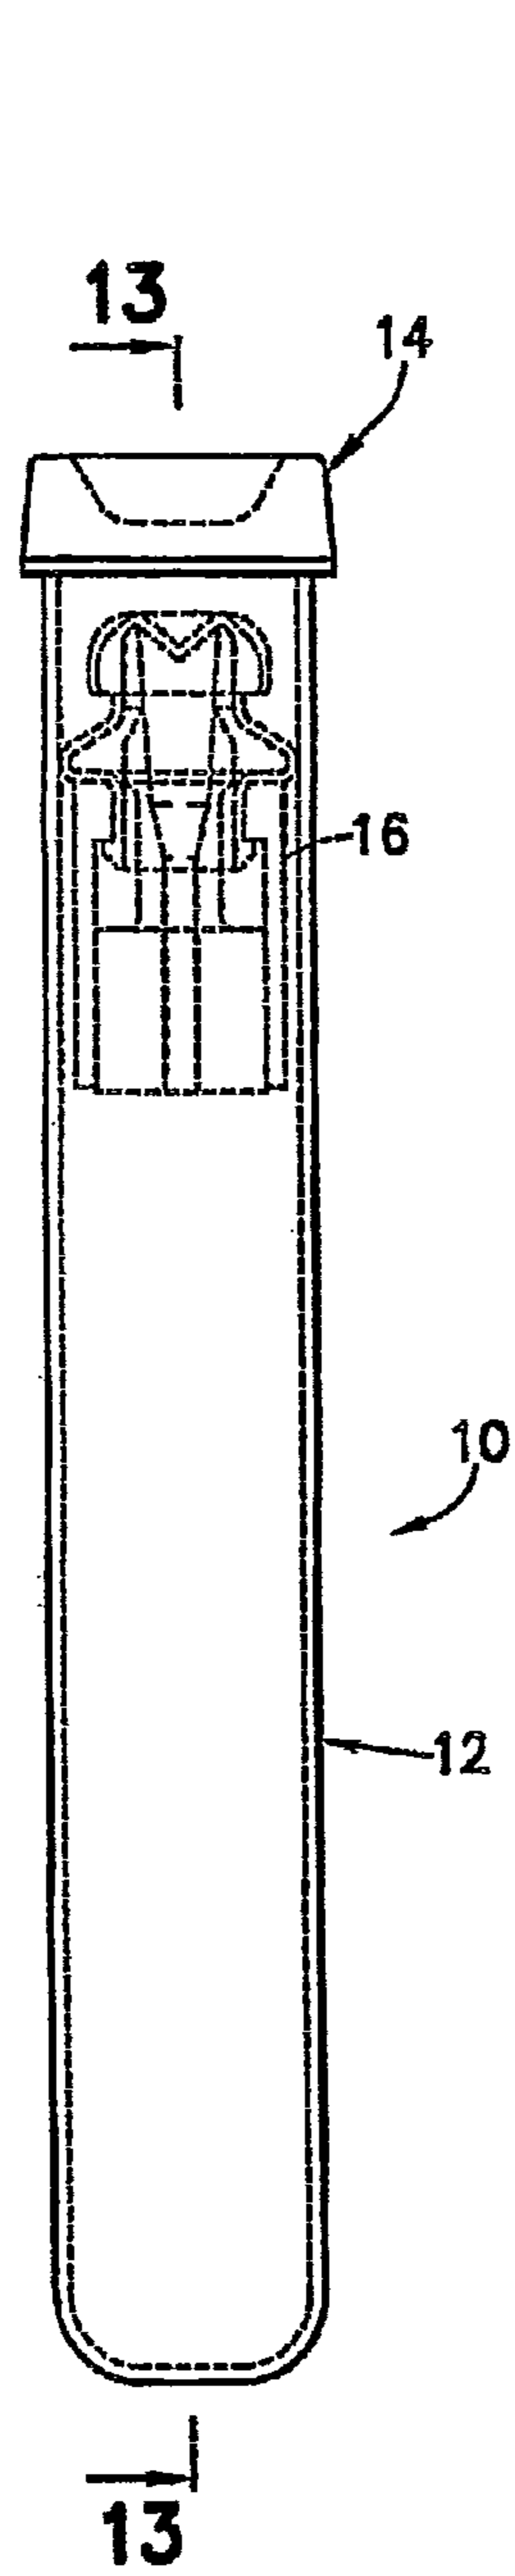


FIG. 12

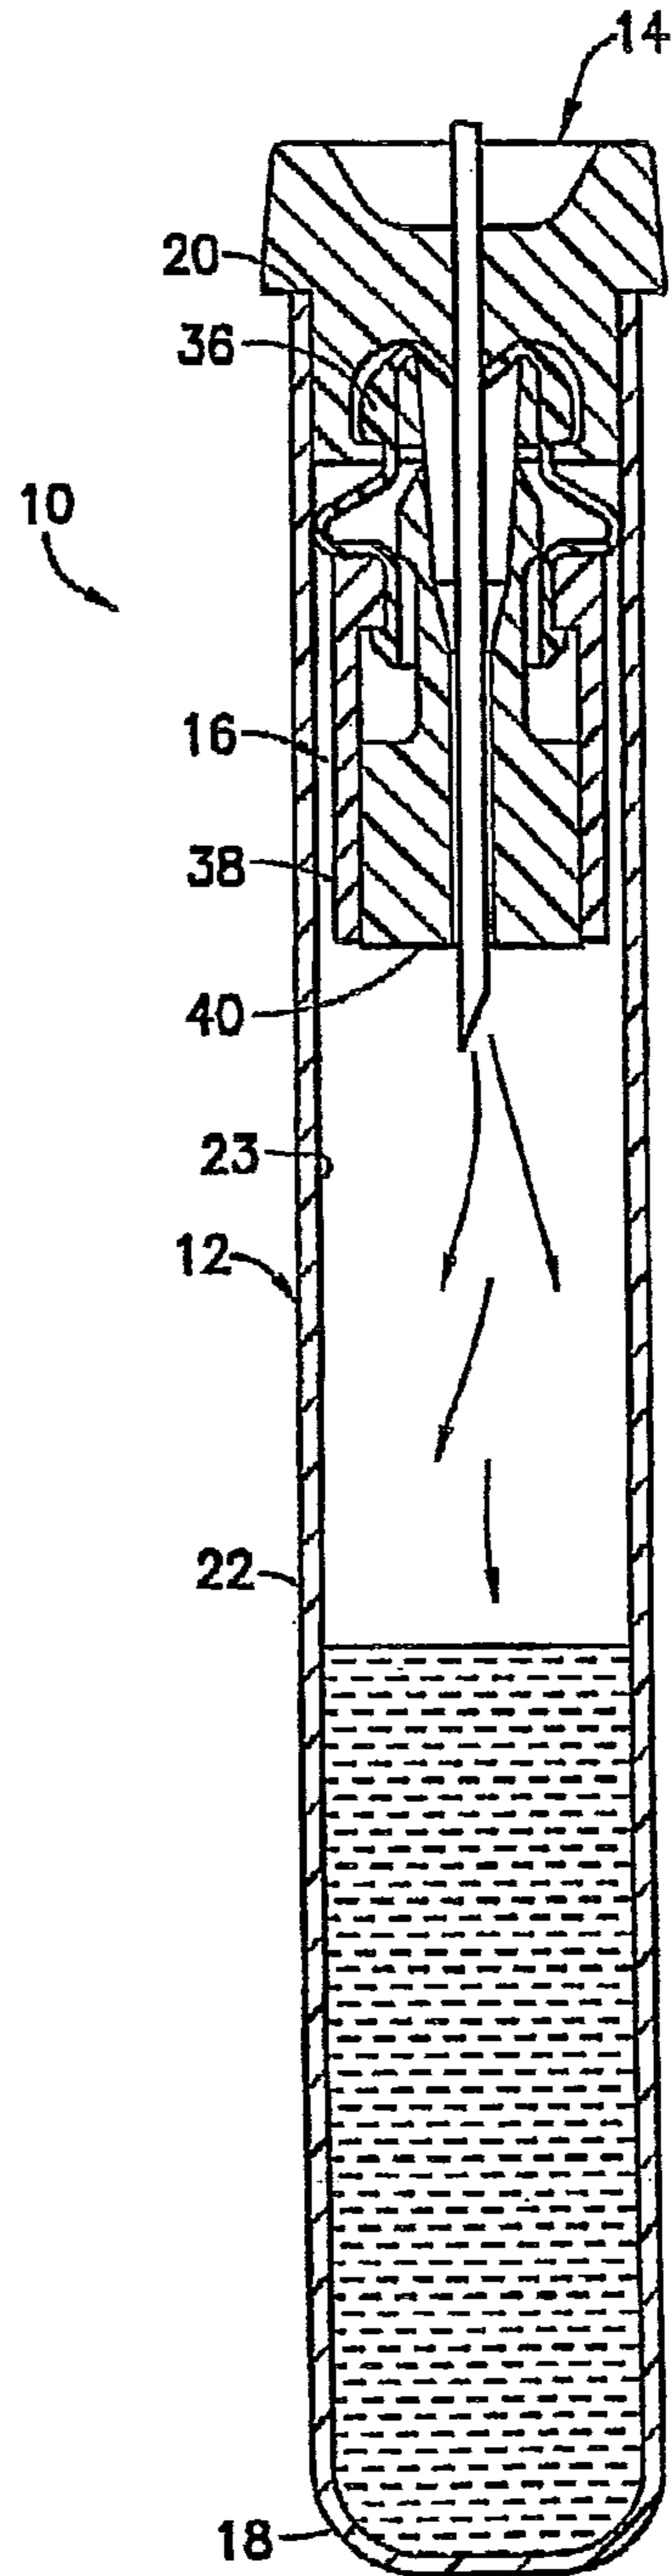


FIG. 13

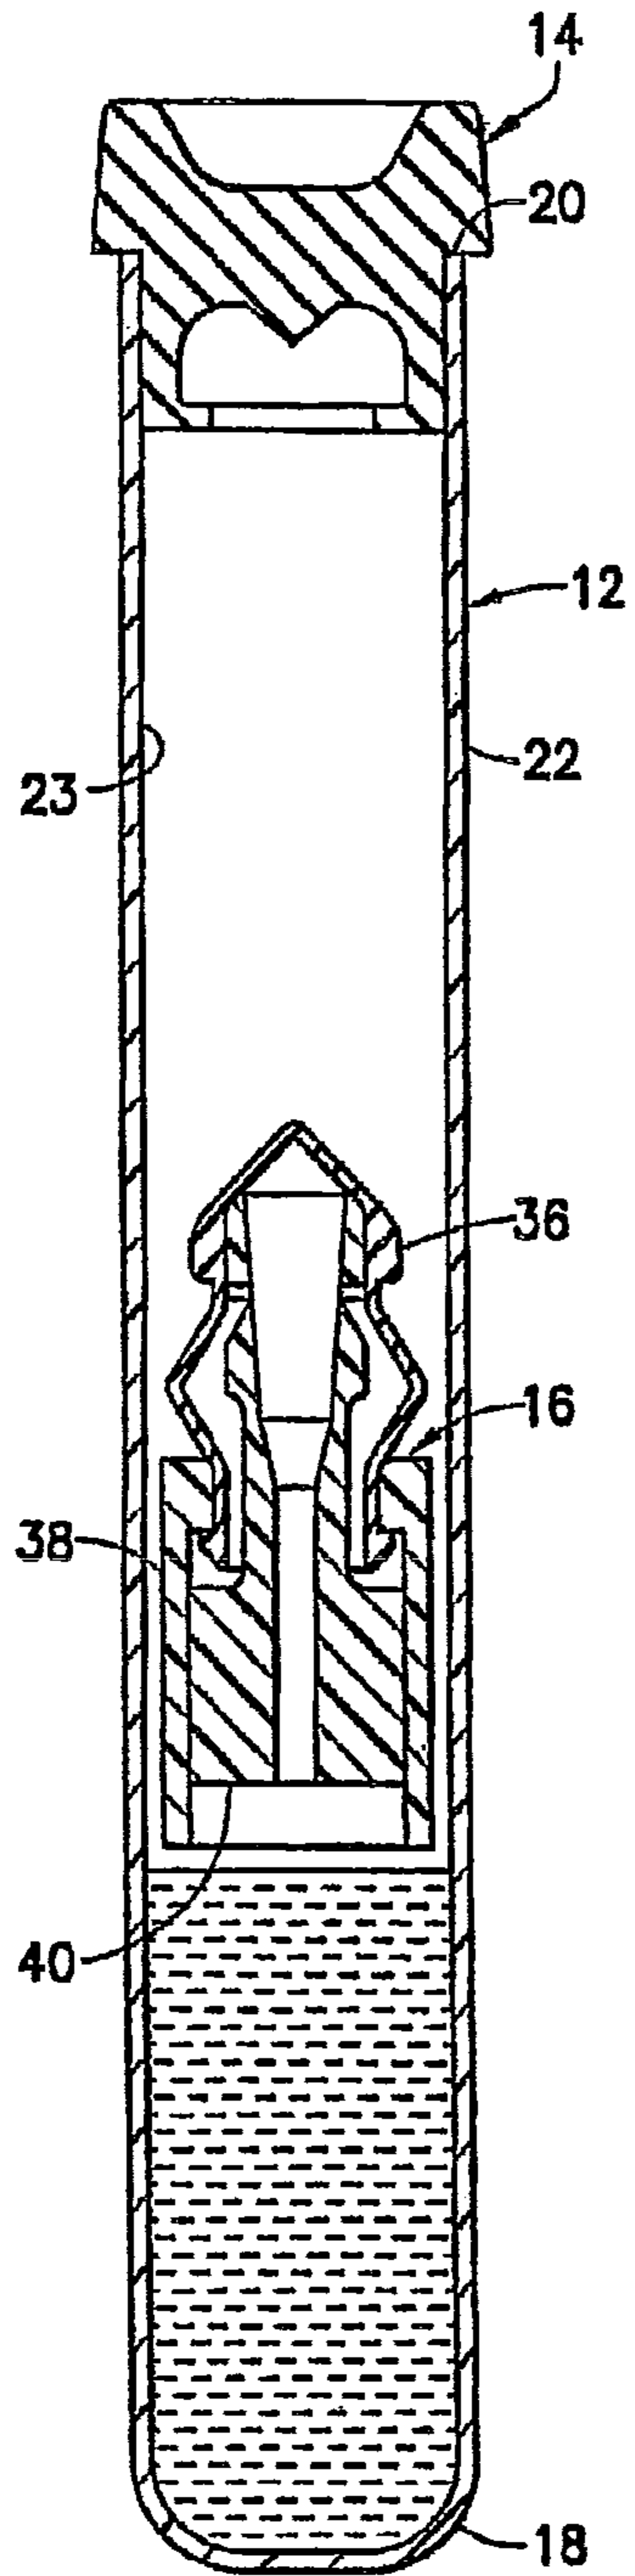


FIG. 14

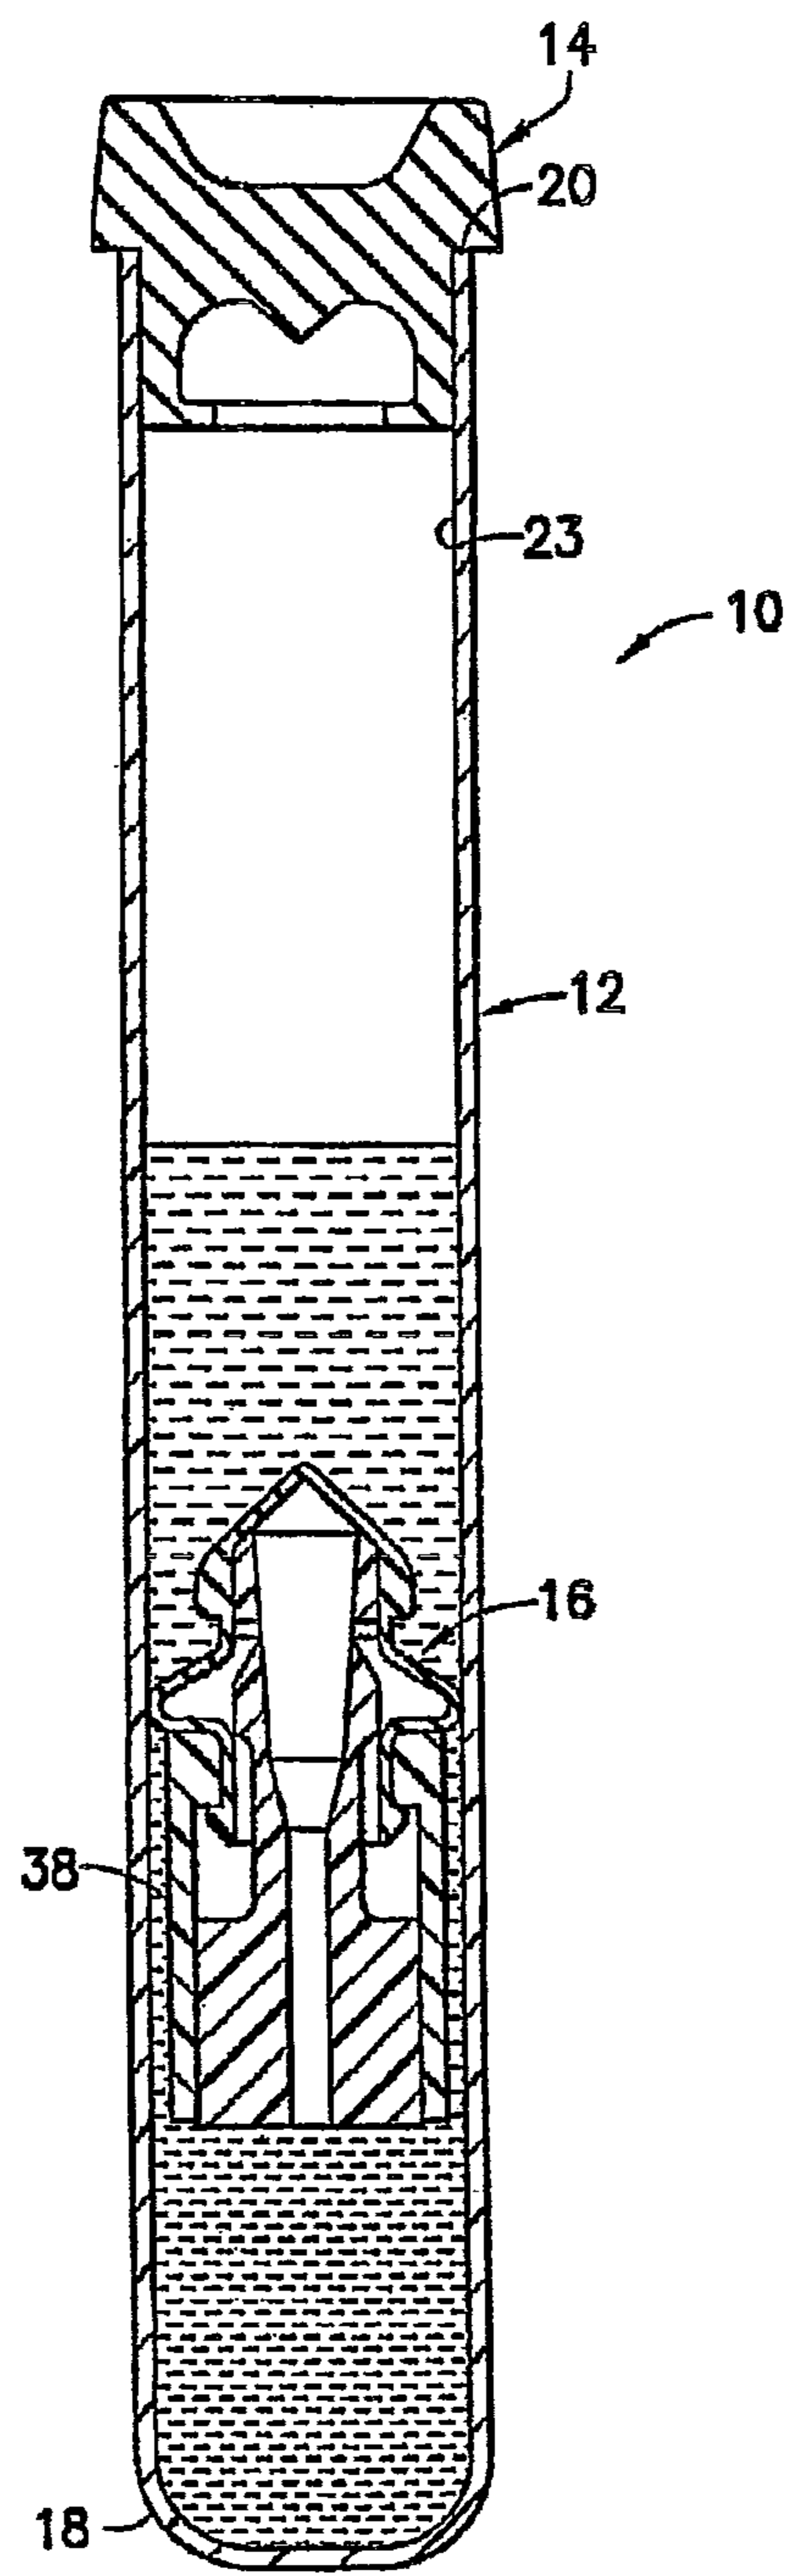


FIG. 15

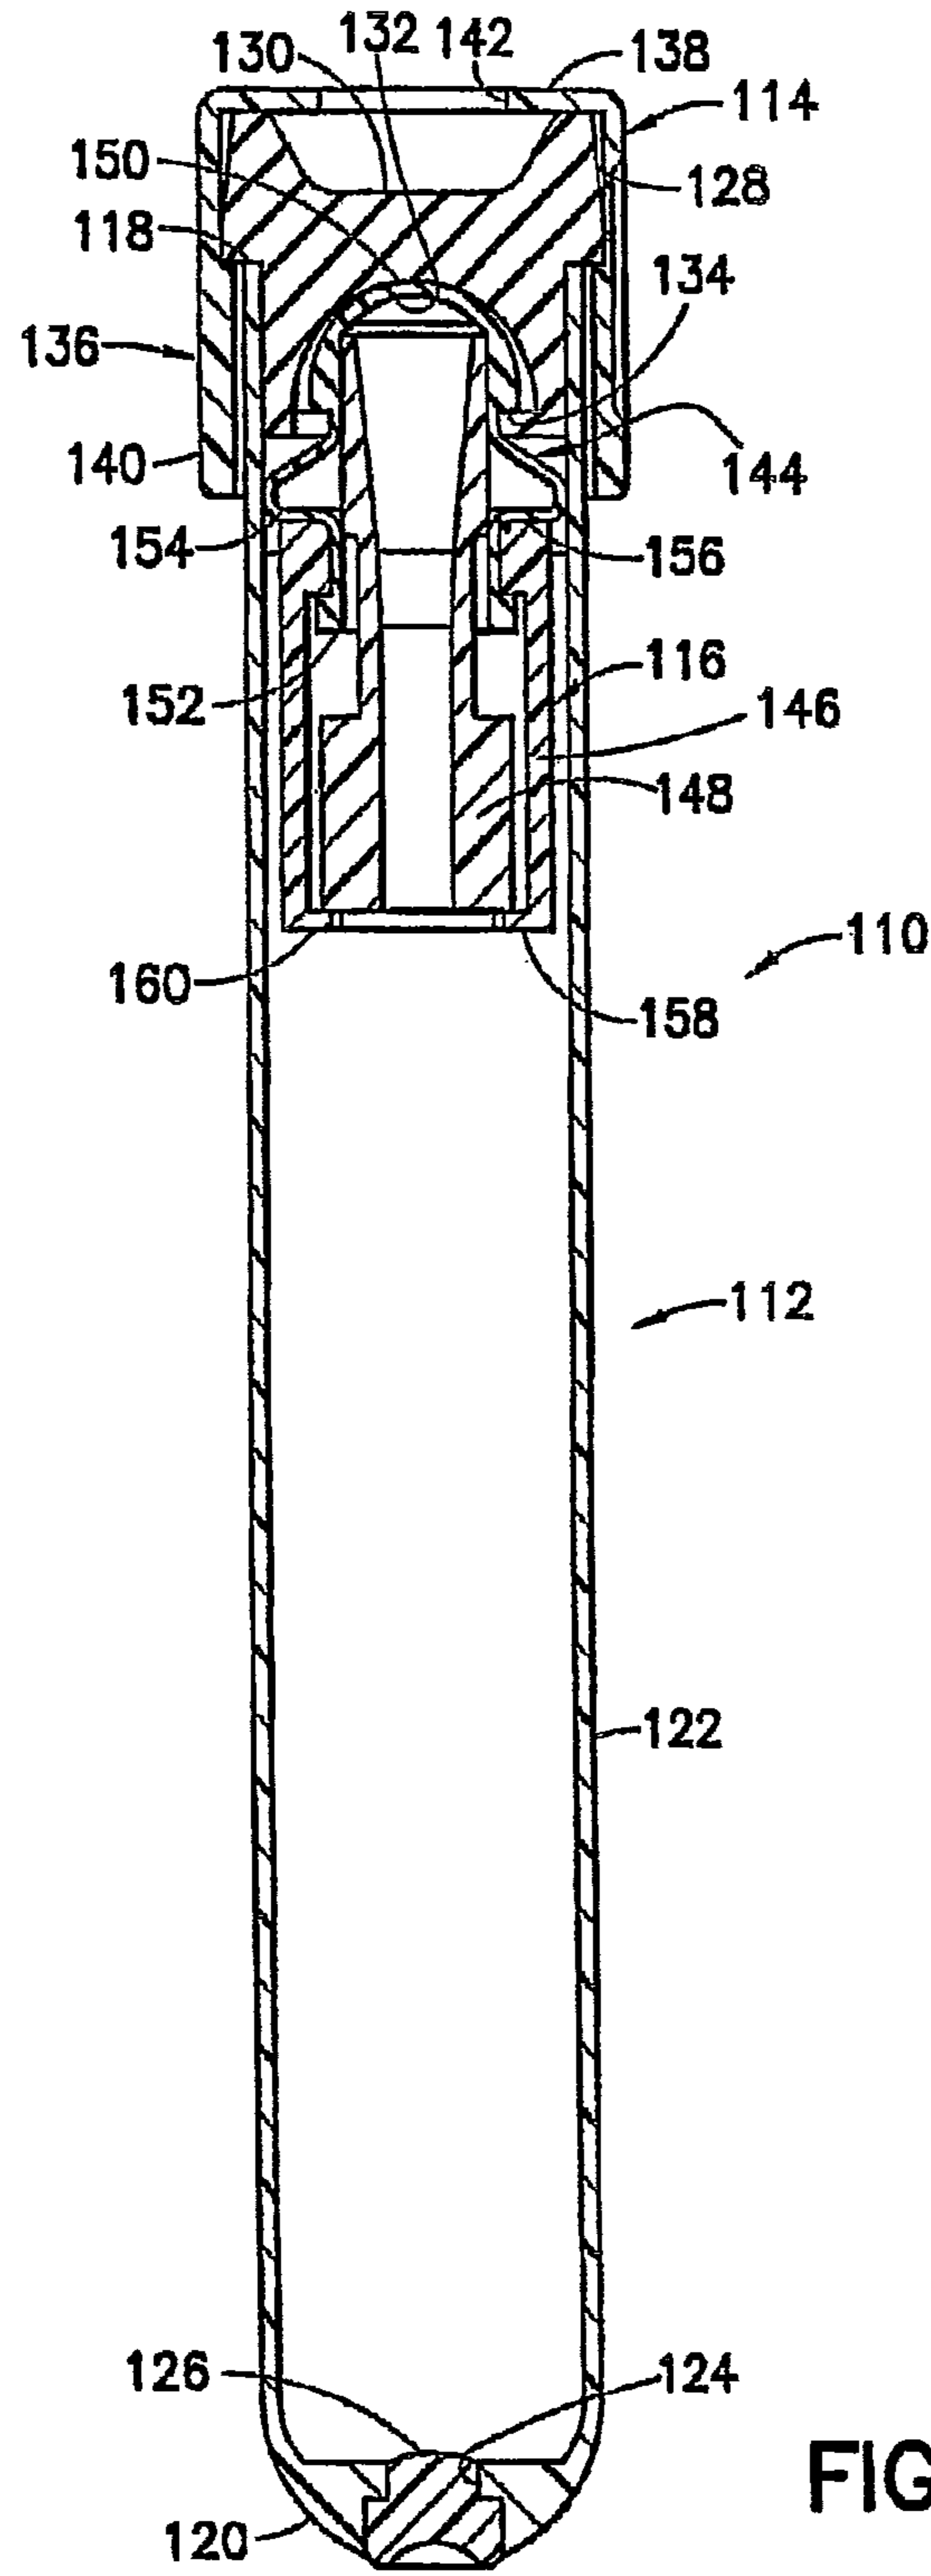


FIG. 16

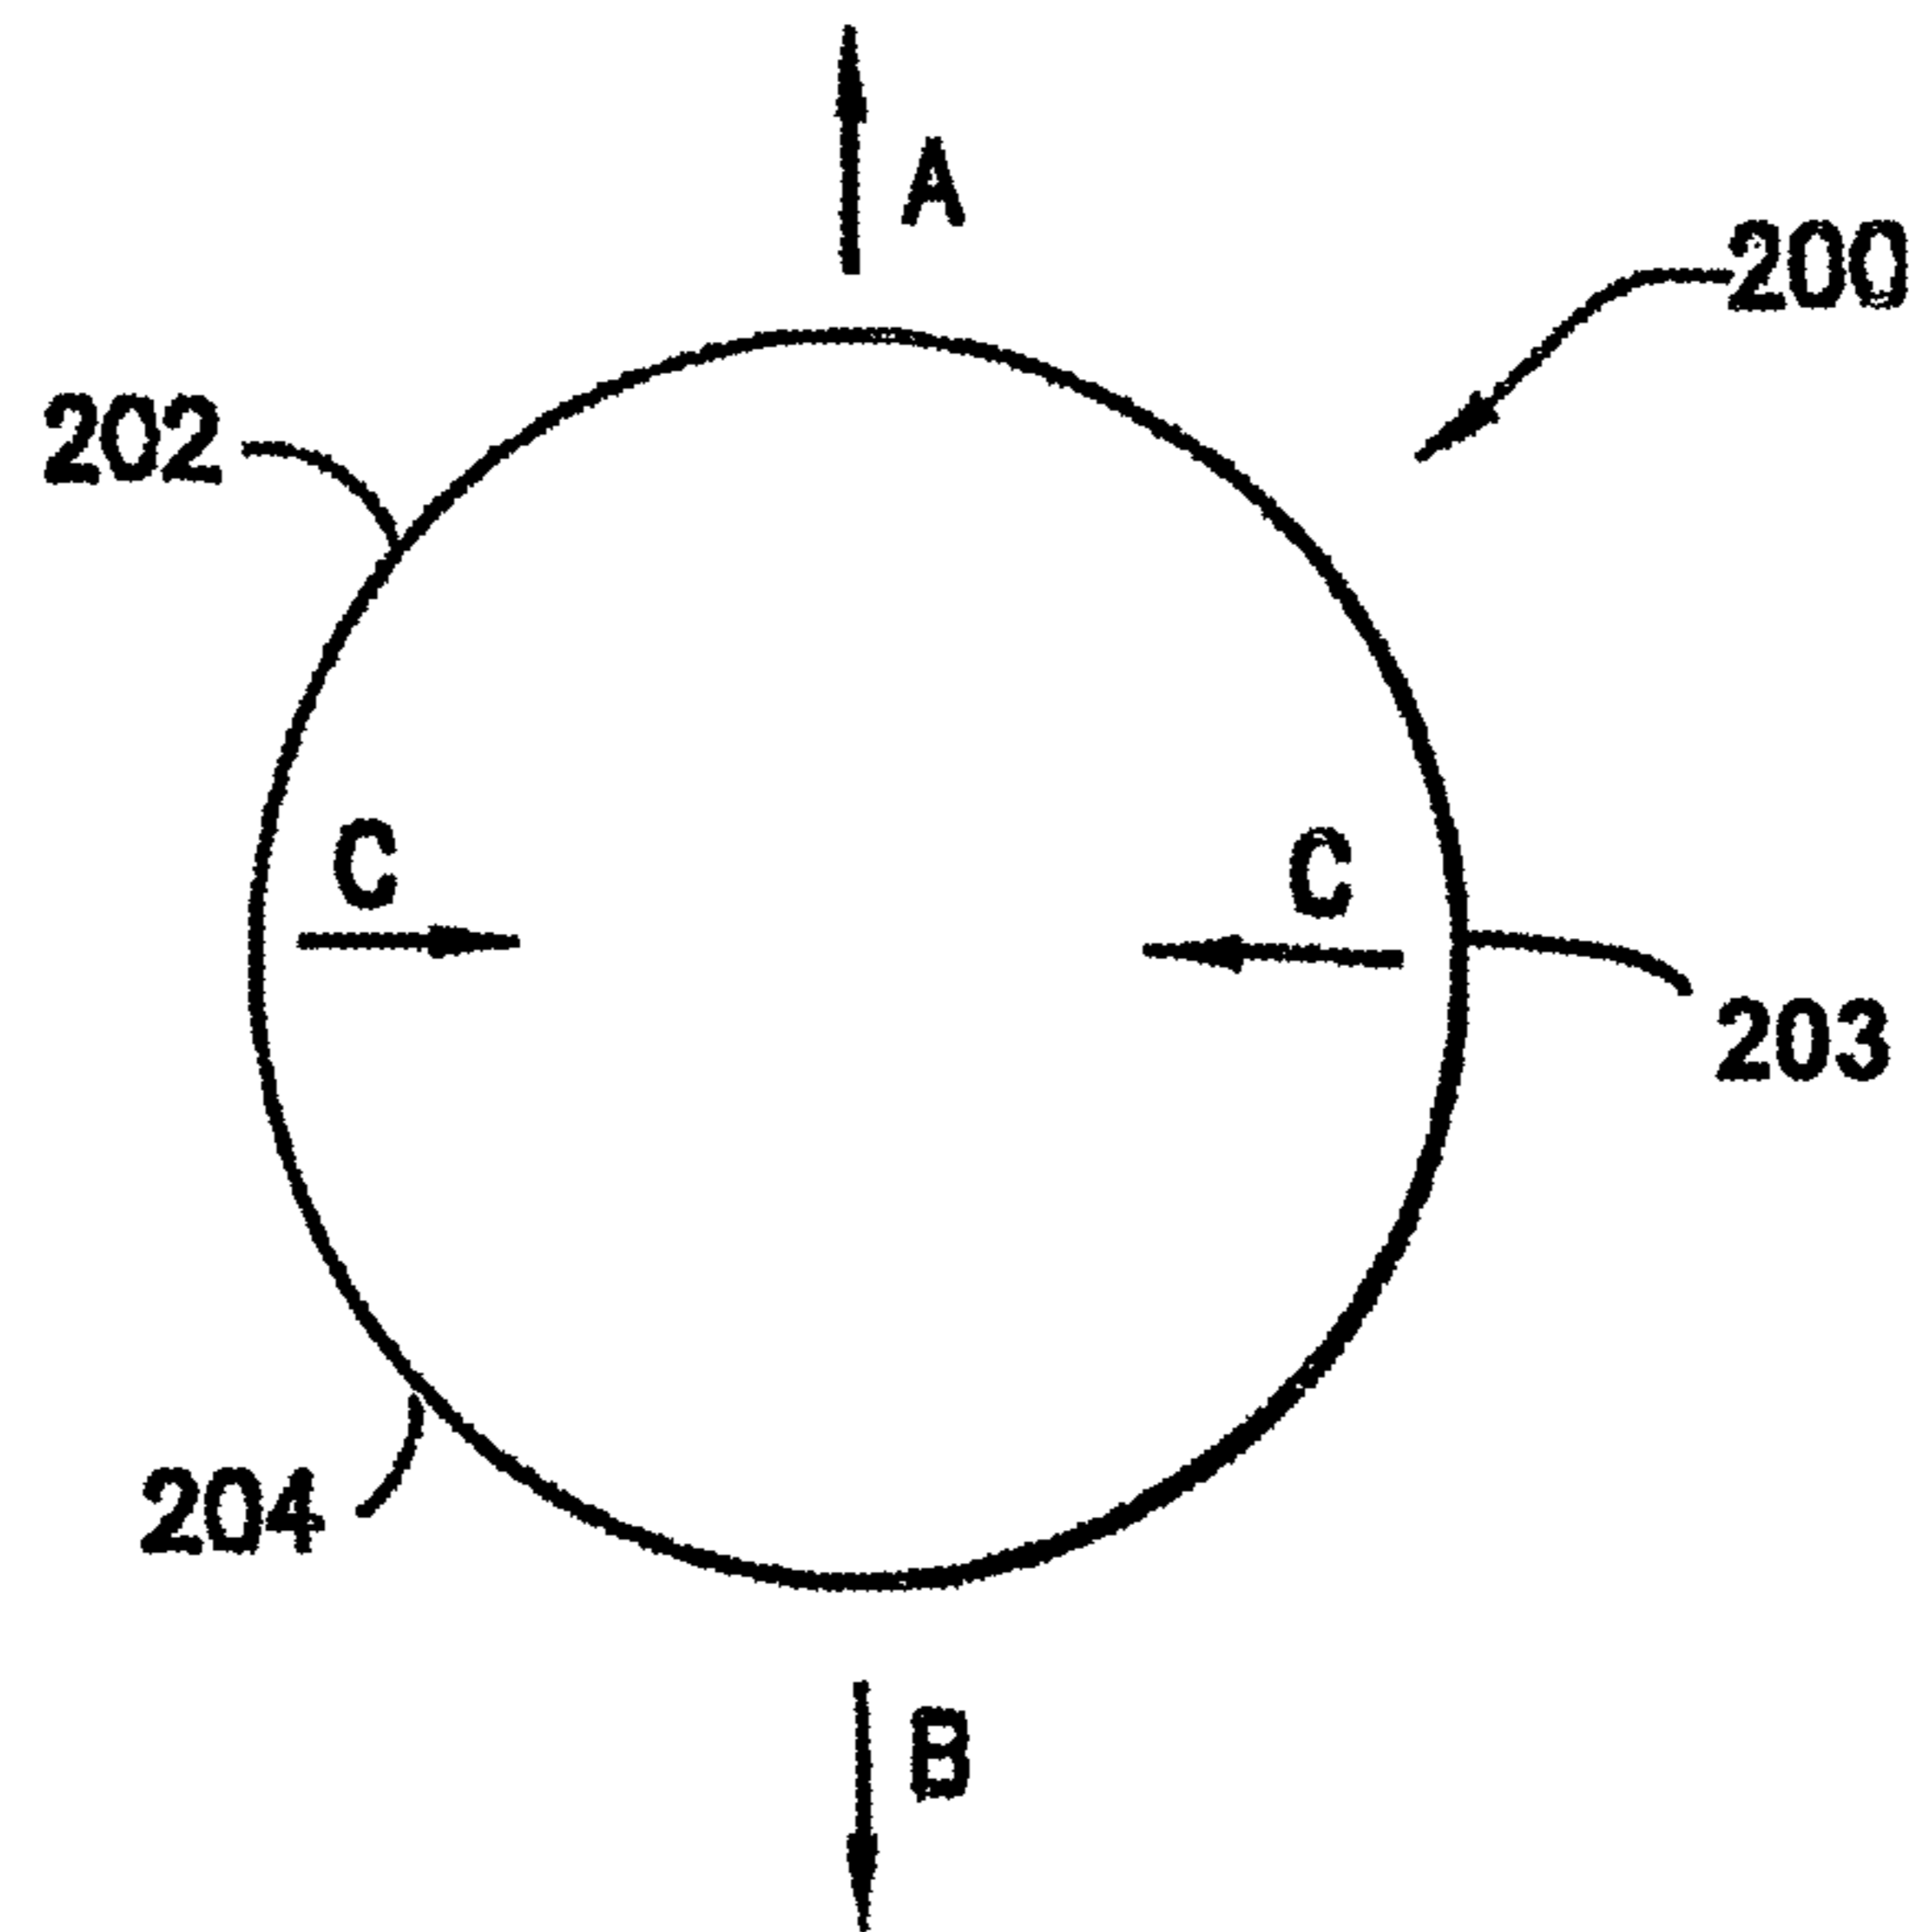


FIG. 17

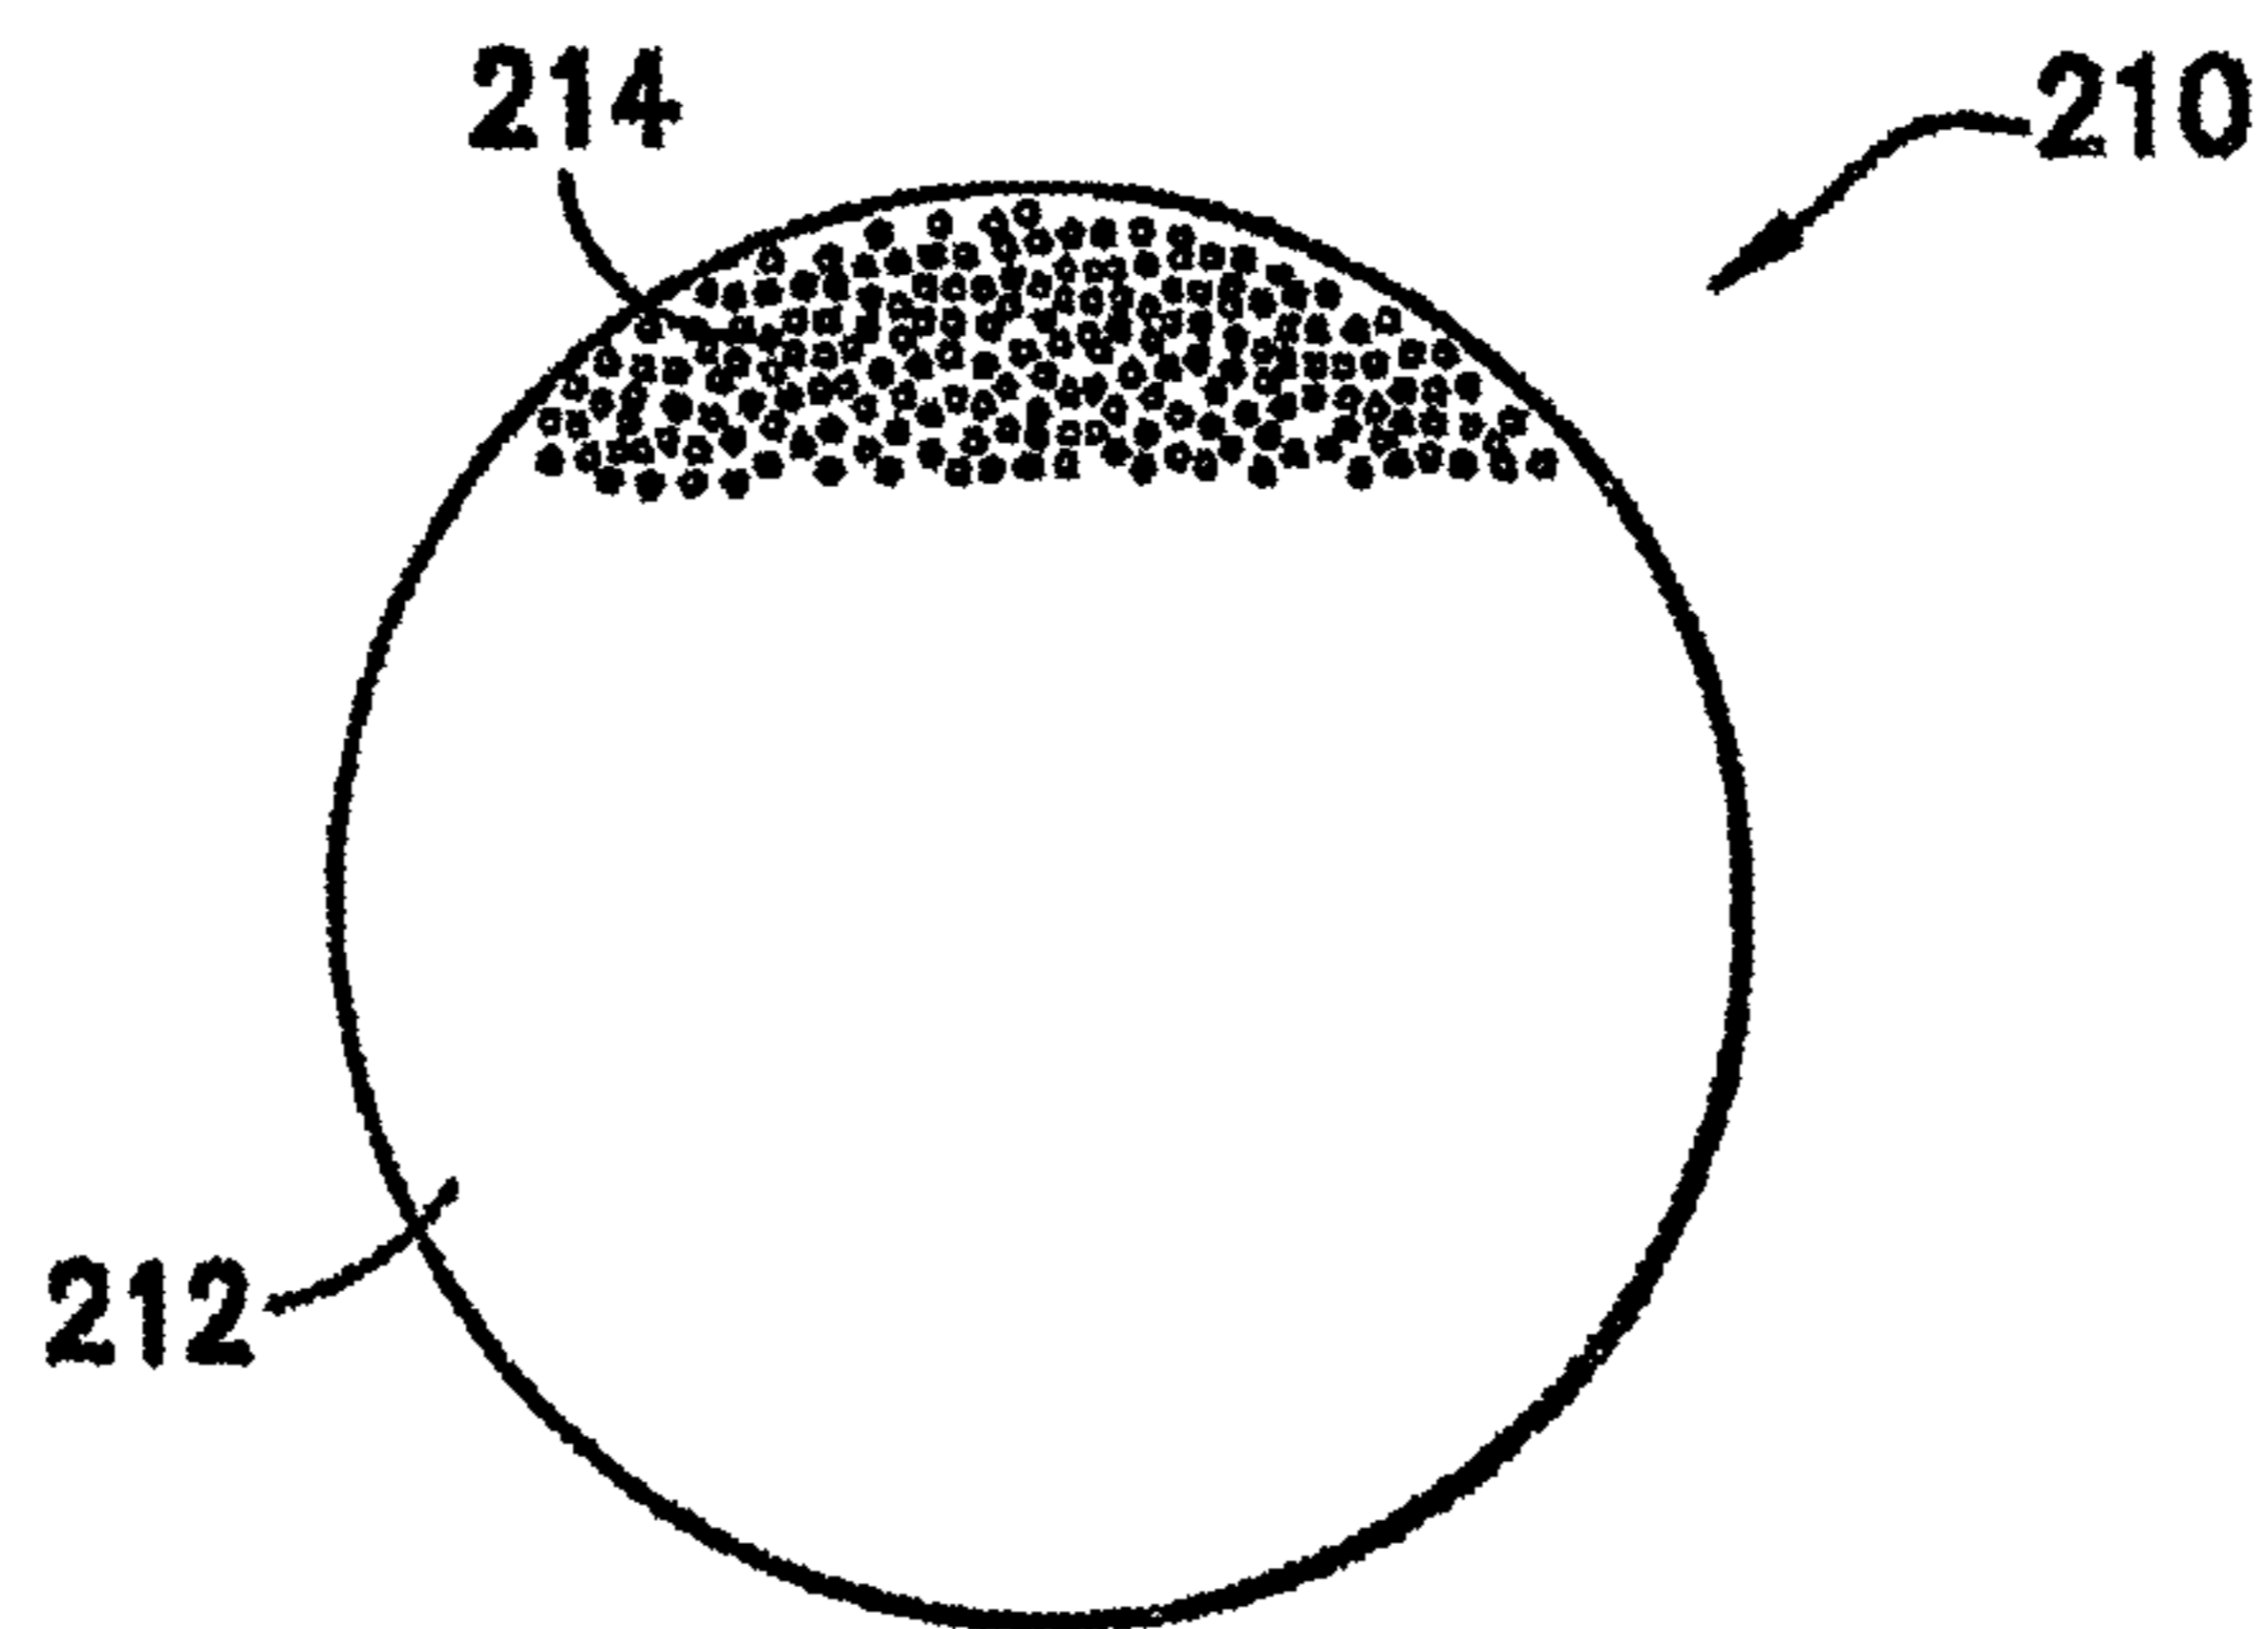


FIG. 18

DEVICE FOR SEPARATING COMPONENTS OF A FLUID SAMPLE

CROSS REFERENCE TO RELATED APPLICATIONS

The present application is a continuation of, and claims priority to, U.S. patent application Ser. No. 13/085,831 filed Apr. 13, 2011, which is a divisional of U.S. patent application Ser. No. 10/785,893, now U.S. Pat. No. 7,947,236, which is a continuation-in-part of U.S. patent application Ser. No. 09/727,282, now U.S. Pat. No. 6,803,022, which is a continuation-in-part of U.S. patent application Ser. No. 09/454,988, now U.S. Pat. No. 6,479,298, the entire disclosures of each of which are hereby incorporated by reference.

BACKGROUND OF THE INVENTION

1. Field of the Invention

This invention relates to a device for separating heavier and lighter fractions of a fluid sample, and in particular a container containing a separator that provides such separation of blood upon centrifugation.

2. Description of Related Art

Diagnostic tests may require separation of a patient's whole blood sample into components such as serum or plasma (a lighter phase component) and red blood cells (a heavier phase component). Samples of whole blood are typically collected by venipuncture through a cannula or needle attached to a syringe or an evacuated collection tube. Separation of the blood into serum or plasma and red blood cells is then accomplished by rotation of the syringe or tube in a centrifuge. The tube or syringe generally contains a barrier that moves between the two phases upon centrifugation, and maintains that separation thereafter to allow subsequent examination of the individual components.

A variety of devices have been used in collection devices to divide the area between the heavier and lighter phases of a fluid sample. The most widely used devices include thixotropic gel materials such as polyester gels in a tube. These devices require special manufacturing equipment to prepare the gel and to fill the tubes. Moreover, the shelf-life of the product may be limited because over time, globules of gel may be released from the gel mass. These globules may enter the serum sample gel and may be released from the gel mass. These globules may enter the serum sample and thereby clog the measuring instruments. Such clogging can lead to considerable downtime for an instrument. In addition, no commercially available gel is completely chemically inert to all analytes. If certain drugs are present in the blood sample when it is taken, there can be an adverse chemical reaction with the gel.

Therefore, a need exists for a separator device that avoids the problems of gels. Such a device advantageously exhibits one or more of the following properties: (i) easily used to separate a blood sample; (ii) largely unaffected by temperature during storage and shipping; (iii) stable to radiation sterilization; (iv) employs the benefits of a thixotropic gel barrier yet avoids the disadvantages of placing a gel in contact with the separated blood components; (v) reduces cross contamination of the heavier and lighter phases of the sample during centrifugation; (vi) reduces adhesion of the lower and higher density materials against the separator device; (vii) able to move into position to form a barrier in less time than conventional methods and devices; (viii) able to provide a clearer specimen with less cell contamination

than conventional methods and devices; and (ix) able to be used with standard sampling equipment.

SUMMARY OF THE INVENTION

The invention relates to an assembly for separating a fluid sample into a higher density phase and a lower density phase. Typically, the assembly comprises a container such as a tube and a separator located in the tube.

A typical tube comprises an open end, a closed end, and a sidewall extending between the open end and closed end. The sidewall comprises an outer surface and an inner surface. The tube further comprises a closure disposed to fit in the open end of the tube, typically with a resealable septum. Alternatively, both ends of the tube may be open, and both ends of the tube may be sealed by elastomeric closures. At least one of the closures of the tube may include a needle pierceable resealable septum.

The separator element comprises an overall density at a target density of σ_r . The target density is required to separate a fluid sample into at least two phases. The separator comprises at least two or more regions of differing densities. Typically, at least one of the regions is higher than the target density and at least one of the regions is lower than the target

density.

In one embodiment, the separator includes opposed top and bottom ends and comprises a bellows, a ballast, and a float. The separator is disposed in the tube at a location between the top closure and the bottom of the tube. The components of the separator are dimensioned and configured to achieve an overall density for the separator that lies between the densities of the phases of a fluid sample, such as a blood sample.

The bellows of the separator is molded from a resiliently deformable material that exhibits good sealing characteristics when placed against an adjacent surface. The bellows has an upper end that is at or in proximity to the top end of the separator and an opposed lower end that is disposed between the opposed ends of the separator.

The upper end of the bellows may be formed from a material that may be pierced by a needle cannula for depositing a fluid sample into the tube. Additionally, the upper end of the bellows initially may be engaged releasably with the closure mounted in the open top end of the tube.

Preferably, the bellows includes a toroidal sealing section which, in an unbiased state of the bellows, defines an outer diameter that exceeds the inside diameter of the tube. However, the bellows can be deformed slightly so that the outer circumferential surface of the toroidal sealing section is biased against the inner circumferential surface of the tube to achieve a sealing engagement between the bellows and the tube. The bellows may be elongated by oppositely directed forces in proximity to the opposed upper and lower ends thereof. Elongation of the bellows in response to such oppositely directed forces will reduce the outside diameter of the toroidal sealing section of the bellows. Sufficient elongation of the bellows will cause the toroidal sealing section of the bellows to be spaced inwardly from the internal surface of the blood collection tube, and thereby allow the separator to move within the tube.

Desirably, the toroidal sealing section may be comprised of any natural or synthetic elastomer or mixture thereof, that is inert to the fluid sample of interest and is flexible.

In use, a fluid sample enters the assembly by needle. Where the separator is secured at the top of the tube, the needle pierces a portion of the bellows adjacent the top end of the separator and partially through the hollow interior of

the float. The needle is withdrawn from the assembly and the septum of the closure and the bellows reseals.

The assembly is then subjected to centrifugation. Forces exerted by the centrifuge causes a gradual separation of the phases of the fluid sample such that the more dense phase moves toward the bottom end of the tube, and the less dense phase is displaced to regions of the tube above the more dense phase. Simultaneously, the centrifugal load will cause the dense ballast to move outwardly relative to the axis of rotation and toward the bottom of the tube. This movement of the ballast will generate an elongation and narrowing of the bellows. Thus, the outside diameter of the toroidal sealing section of the bellows will become less than the inside diameter of the tube. Additionally, the centrifugal load and the deformation of the bellows will cause the separator to disengage from the top closure. Hence, the separator will begin to move toward the bottom of the tube. Air trapped between the fluid sample and the separator initially will move through the circumferential space between the separator and the tube. After sufficient movement, the bottom end of the separator will contact the surface of the fluid sample. At this point, air trapped within the hollow interior of the separator can impede further downward movement of the separator into the fluid sample. However, this air can pass through the defect in the bellows caused by the needle or through some other manufactured defect in the bellows.

The ballast will cause the separator to sink into the fluid sample while the float will buoyantly remain near the surface of the fluid sample thereby causing an elongation and narrowing of the bellows. The less dense liquid phase of the fluid sample will move through the space between the separator and the walls of the tube. As noted above, the overall density of the separator is selected to be less than the density of the formed phase of the fluid sample, but greater than the density of the less dense liquid phase of the fluid sample. Thus, the separator will stabilize at a location between the foamed and liquid phases of the fluid sample after a sufficient period of centrifugation. The centrifuge then is stopped. The termination of the centrifugal load enables the toroidal sealing section of the bellows to return toward its unbiased dimensions, and into sealing engagement with the interior of the tube. The less dense liquid phase of the fluid sample can be separated from the tube by either removing the closure or passing a needle through the closure. Alternatively, in certain embodiments, the more dense formed phase can be accessed through a sealed opening in the bottom end of the tube.

In another embodiment, it is possible for the separator element to be a unitary structure having regions of different densities that provide, for example, the functionality of the buoyancy member and ballast member discussed herein. (Unitary indicates a single mechanical component versus a combination of mechanical components, with the single mechanical component made up of one or more materials.) For example, it is possible for the separator element to be a sphere-like element formed from a polymeric material, where the upper region of the element comprises a relatively low density material, and the lower region contains a relatively high density material. (The separator may have a density gradient, such that distinct regions of uniform density may not exist, but portions of the separator will have different average densities.) Upon centrifugation, the low and high density regions would act as the buoyancy and ballast members, respectively, with at least a portion of the region therebetween acting as a sealing member.

It is possible to obtain the high and low density regions by a variety of techniques, including molding a high density

elastomeric matrix with low density components, including air bubbles or voids, distributed at an upper region therein (to provide buoyancy), or to mold a low density elastomeric matrix with high density components distributed at a lower region therein (to provide ballast). It is also possible to co-mold two or more different materials (or the same materials but having different densities) to provide the distinct densities.

The assembly of the invention is advantageous over existing separation products that use gel. For example, the separator of the invention will not interfere with analytes as compared to gels that may do so, nor will the separator of the invention interfere with therapeutic drug monitoring analytes. Other advantages that the separator may provide over gel include reduced separation time, avoidance of gel residuals, no interference with instrument probes, more acceptable blood banking tests, and a cleaner sample (where the blood is initially provided beneath the separator) due to the fact that only the cell-free fraction contacts the upper portion of the separator.

DESCRIPTION OF THE DRAWINGS

FIG. 1 is an exploded perspective view of an assembly of one embodiment of the invention.

FIG. 2 is a perspective view of the closure of the assembly of FIG. 1.

FIG. 3 is a bottom plan view of the closure of FIG. 2.

FIG. 4 is a cross-sectional view of the closure of FIG. 3 thereof.

FIG. 5 is a perspective view of the bellows of the separator of the assembly of FIG. 1.

FIG. 6 is a cross-sectional view of the bellows of FIG. 5 taken along line 6-6 thereof.

FIG. 7 is a bottom plan view of the ballast of the separator of the assembly of FIG. 1.

FIG. 8 is a cross-sectional view of the ballast of FIG. 7 taken along line 8-8 thereof.

FIG. 9 is a perspective view of the float of the separator of the assembly of FIG. 1.

FIG. 10 is a side elevational view of the float of the separator of the assembly of FIG. 1.

FIG. 11 is a cross-sectional view of the float of FIG. 10 taken along line 11-11 thereof.

FIG. 12 is a side elevational view of an assembly of an embodiment of the invention.

FIG. 13 is a cross-sectional view of the assembly of FIG. 12 taken along line 13-13 thereof.

FIG. 14 is a cross-sectional view of the assembly of FIG. 12 taken along line 13-13 thereof, showing the separator under a centrifugal load.

FIG. 15 is a cross-sectional view of the assembly of FIG. 12 taken along line 13-13 thereof, showing the separator sealingly engaged with the tube between the liquid and formed phases of the fluid sample.

FIG. 16 is a cross-sectional view similar to FIG. 13, but showing an alternate embodiment of the invention.

FIG. 17 illustrates a further embodiment of the invention.

FIG. 18 illustrates another embodiment of the invention.

DETAILED DESCRIPTION

In one embodiment, the separator includes opposed top and bottom ends and comprises a bellows, a ballast, and a float. The separator is disposed in the tube at a location between the top closure and the bottom of the tube. The components of the separator are dimensioned and configured

5

to achieve an overall density for the separator that lies between the densities of the phases of a fluid sample, such as a blood sample.

The bellows of the separator is molded from a resiliently deformable material that exhibits good sealing characteristics when placed against an adjacent surface. The bellows has an upper end that is at or in proximity to the top end of the separator, and an opposed lower end that is disposed between the opposed ends of the separator.

The upper end of the bellows may be formed from a material that may be pierced by a needle cannula for depositing a fluid sample into the tube. Additionally, the upper end of the bellows initially may be engaged releasably with the closure mounted in the open top end of the tube.

Preferably, the bellows includes a toroidal sealing section which, in an unbiased state of the bellows, defines an outer diameter that exceeds the inside diameter of the tube. However, the bellows can be deformed slightly so that the outer circumferential surface of the toroidal sealing section is biased against the inner circumferential surface of the tube to achieve a sealing engagement between the bellows and the tube. The bellows may be elongated by oppositely directed forces in proximity to the opposed upper and lower ends thereof. Elongation of the bellows in response to such oppositely directed forces will reduce the outside diameter of the toroidal sealing section of the bellows. Sufficient elongation of the bellows will cause the toroidal sealing section of the bellows to be spaced inwardly from the internal surface of the blood collection tube.

Desirably, the toroidal sealing section may be comprised of any natural or synthetic elastomer or mixture thereof, that is inert to the fluid sample of interest and is flexible.

Preferably, the toroidal sealing section comprises a qualitative stiffness, expressed as follows: $S^*=K/(a\rho_w D^2)$

whereby "S*" is the non-dimensional stiffness coefficient, "k" is a force required to deflect the bellows a given length, "a" is the applied acceleration, "D" is the diameter of the toroidal sealing section, and " ρ_w " is the density of water.

Desirably, the qualitative stiffness of the toroidal sealing section is from about 0.00006 to about 190.

Preferably, the toroidal sealing section may be subjected to a characteristic or radial deflection under an applied load such as an axially applied load. The characteristic or radial deflection is defined as a change in length of the toroidal sealing section relative to the change in cross section diameter of the toroidal sealing section. Preferably, the toroidal sealing section has a characteristic or radial deflection ratio of about 1.5 to about 3.5.

Preferably, the toroidal sealing section when subjected to an applied load, such as centrifugation, to cause axial deformation of the toroidal sealing section, the change in cross section diameter of the toroidal sealing section may be expressed as follows: $((D_{before}-D_{during})/D_{before})\times 100\%=\Delta D_m$

wherein " ΔD_m " is from about 5% to about 20%.

Therefore, a change in cross section diameter of the toroidal sealing section is proportional to the undeflected cross section diameter of the toroidal sealing section. Preferably, the proportion is from about 0.03 to about 0.20.

In this embodiment, the ballast is a substantially tubular structure formed from a material having a greater density than the heavy phase of blood. The generally tubular ballast has a maximum outside diameter that is less than the inside diameter of the tube. Hence, the ballast can be disposed concentrically within and spaced from a cylindrical sidewall of the tube. The ballast may be securely and permanently mounted to the lower end of the bellows.

6

In this embodiment, the float is formed from a material having a density less than the density of the lighter phase of the blood and may be engaged near the upper end of the bellows. Additionally, the float is movable relative to the ballast. For example, the float may be substantially tubular and may be slidably telescoped concentrically within the tubular ballast. Hence, the float and the ballast can move in opposite respective directions within the tube.

In use, a fluid sample enters the assembly by needle. Where the separator is secured at the top of the tube, the needle pierces a portion of the bellows adjacent the top end of the separator and partially through the hollow interior of the float. The needle is withdrawn from the assembly and the septum of the closure and the bellows reseals.

The assembly is then subjected to centrifugation. Forces exerted by the centrifuge causes a gradual separation of the phases of the fluid sample such that the more dense phase moves toward the bottom end of the tube, and the less dense liquid is displaced to regions of the tube above the more dense phase. Simultaneously, the centrifugal load will cause the dense ballast to move outwardly relative to the axis of rotation and toward the bottom of the tube. This movement of the ballast will generate an elongation and narrowing of the bellows. Thus, the outside diameter of the toroidal sealing section of the bellows will become less than the inside diameter of the tube. Additionally, the centrifugal load and the deformation of the bellows will cause the separator to disengage from the top closure. Hence, the separator will begin to move toward the bottom of the tube. Air trapped between the fluid sample and the separator initially will move through the circumferential space between the separator and the tube. After sufficient movement, the bottom end of the separator will contact the surface of the fluid sample. At this point, air trapped within the hollow interior of the separator can impede further downward movement of the separator into the fluid sample. However, this air can pass through the defect in the bellows caused by the needle or through some other manufactured defect in the bellows.

The ballast will cause the separator to sink into the fluid sample while the float will buoyantly remain near the surface of the fluid sample thereby causing an elongation and narrowing of the bellows. The less dense liquid phase of the fluid sample will move through the space between the separator and the walls of the tube. As noted above, the overall density of the separator is selected to be less than the density of the formed phase of the fluid sample, but greater than the density of the less dense liquid phase of the fluid sample. Thus, the separator will stabilize at a location between the formed and liquid phases of the fluid sample after a sufficient period of centrifugation. The centrifuge then is stopped. The termination of the centrifugal load enables the toroidal sealing section of the bellows to return to its unbiased dimensions, and into sealing engagement with the interior of the tube. The less dense liquid phase of the fluid sample can be separated from the tube by either removing the closure or passing a needle through the closure. Alternatively, in certain embodiments, the more dense formed phase can be accessed through a sealed opening in the bottom end of the tube.

The separator of the invention comprises a useful range of parameters and there are two principle driving equations for defining the parameters:

$$\sigma_i V_i = \sigma_f V_f + \sigma_s V_s$$

65 Conservation of Mass

$$((\sigma_f - \sigma_i) V_f - (\sigma_s - \sigma_i) V_s) \rho_w = (\delta \cdot \Delta D \cdot k) / a$$

Force Balance

The following non-dimensional parameters may then be substituted into the force balance:

$$V_s^*=V_s/D^3, V_f^*=V_f/D^3; S^*=k/a \rho_w D^2$$

to arrive at:

$$(\sigma_f - \sigma_t)V_g^* - (\sigma_s - \sigma_t)V_s^* = (\delta \Delta D \cdot S^*)/D$$

So as to scale prototypes to any size device, wherein the following are defined:

" σ_t ", " σ_f ", " σ_s ", are the specific gravities of the separator device, float, and ballast, respectively;

" V_t ", " V_f ", " V_s " are the volumes of the separator device, float, and ballast, respectively;

" ρ_w " is the density of water;

" k " is the separator spring constant;

" a " is the applied acceleration; and

the deflection ration defined by: $\Delta L/\Delta D$, where " ΔL " is the change in length.

The left side of the equation can be an infinite number of combinations of materials and geometries and if it is equal to the product of the right side it can be concluded that the device will function.

Desirable values for the right side of the equation are as follows:

$$\delta = 1.5 - 3.5$$

$$\Delta D/D = 0.05 \text{ to } 0.2$$

$$S^* = 0.043 \text{ to } 0.220.$$

One embodiment of the invention is illustrated in FIGS. 1 and 13-15, wherein assembly 10 includes a tube 12, a closure 14, and a separator assembly 16. Tube 12 includes a closed bottom 18, an open top 20, and a cylindrical sidewall 22 extending therebetween. Sidewall 22 includes an inner surface 23 with an inside diameter "a" extending from top end 20 to a location substantially adjacent bottom end 18.

Closure 14, as shown in FIGS. 2-4, is unitarily molded from an elastomeric material and includes a top end 24 and a bottom end 26. Portions of closure 14 adjacent top end 24 define a maximum outside diameter which exceeds the inside diameter "a" of tube 12. Additionally, portions of closure 14 at top end 24 include a central recess 28 which defines a needle pierceable resealable septum. Portions of closure 14 extending upwardly from bottom end 26 taper from a minor diameter which is approximately equal to or slightly less than the inside diameter "a" of tube 12 to a major diameter that is greater than inside diameter "a". Thus, bottom end 26 of closure 14 can be urged into portions of tube 12 adjacent open top end 20 thereof, and the inherent resiliency of closure 14 will ensure a sealing engagement with the inner circumferential surface of cylindrical sidewall 22 of tube 12.

Closure 14 is formed to include a bottom recess 30 extending into bottom end 26. Bottom recess 30 is characterized by a central convex cone 32. Additionally, a plurality of spaced apart resiliently deflectable arcuate flanges 34 extend around the entrance to recess 30. Flanges 34 function to releasably hold separator assembly 16.

Separator assembly 16 includes a bellows 36, a ballast 38, and a float 40. Bellows 36, as shown in FIGS. 5 and 6, is unitarily molded from a resiliently deformable material, that exhibits good sealing characteristics. More particularly, bellows 36 is symmetrical about a center axis and includes an upper end 42, a lower end 44, and a hollow interior 45 that is open at lower end 44. Portions of bellows 36 adjacent upper end 42 define an enlarged mounting head 46 with a top

section that is convexly conical in an initial unbiased condition of bellows 36. The conical section of bellows 36 adjacent upper end 42 can be deflected into a conical concave configuration that abuts conical portion 32 in recess 30 of closure 14. Bellows 36 further includes a generally toroidal sealing section 47 with intermediate upper and lower ends 42 and 44. Toroidal sealing section 47 defines an outside diameter "b" which, in an unbiased condition of bellows 36, slightly exceeds inside diameter "a" of tube 12. However, oppositely directed forces on upper and lower ends 42 and 44 of bellows 36 will lengthen bellows 36 simultaneously reducing the diameter of toroidal sealing section 47 to a dimension less than "a". A narrow neck 48 is defined between mounting head 46 and toroidal sealing section 47. Neck 48 is dimensioned to be engaged within the area defined by arcuate flanges 34 on closure 14. Hollow interior 45 of bellows 36 includes an annular float mounting bead 49 at a location substantially aligned with neck 48.

Portions of bellows 36 between toroidal sealing section 47 and lower end 44 define a generally cylindrical ballast mounting section 50 of outside diameter "c", inside diameter "d," and length "e". Ballast mounting section 50 terminates at an outwardly projecting flange 51 substantially adjacent lower end 44 of bellows 36.

Ballast 38 of separator 16 is generally a cylindrical tube unitarily formed from a material that will not react with blood or other liquid being separated and that has a density higher than the blood or other liquid being separated. Ballast 38 preferably is substantially tubular and includes opposed upper and lower ends 52 and 54, as shown in FIGS. 7 and 8. Outer circumferential surface areas of ballast 38 define a maximum outside diameter "f" that is less than inside diameter "a" of tube 12. Inner circumferential surface regions of ballast 38 are characterized by an inwardly directed flange 56 adjacent upper end 52. Flange 56 defines an inside diameter "g" which is approximately equal to outside diameter "c" of ballast mounting section 50 of bellows 36. Additionally, flange 56 of ballast 38 defines a length "h" which is approximately equal to length "e" of ballast mounting section 50 on bellows 36. As a result, ballast 38 can be securely mounted to ballast mounting section 50 of bellows 36 at locations between flange 51 and toroidal sealing section 47. Portions of ballast 38 between flange 56 and lower end 54 of ballast 38 will project downwardly below lower end 44 of bellows 36 in this interengaged position.

Float 40 of separator 16 is a generally stepped tubular structure unitarily molded from a foam material having a density less than the density of the liquid phase of blood. Float 40 may be unitarily formed from a low density polyethylene. As shown in FIGS. 9-11, float 40 has an upper end 58, a lower end 60, and a passage 62 extending axially therebetween. Float 40 is formed with an annular groove 64 extending around the outer circumferential surface thereof at a location spaced slightly from upper end 58. Annular groove 64 is dimensioned to be resiliently engaged by inwardly directed annular bead 49 of bellows 36 for securely retaining portions of float 40 near upper end 58 to portions of bellows 36 near lower end 44 thereof. Additionally, groove 64 is configured to define apertures 65 that enable an air flow that insures narrowing of bellows 36 in the assembled condition of separator 16, as explained below.

Float 40 further includes narrow neck 66 at locations approximately midway between top and bottom ends 58 and 60. Neck 66 defines a diameter "i" which is less than inside diameter "d" of ballast mounting section 50 of bellows 36.

As a result, neck 66 is freely movable in an axial direction within ballast mounting section 50 of bellows 36.

Float 40 further includes a substantially cylindrical base 68 defining a diameter "j" which is less than the inside diameter of ballast 38 between flange 56 and lower end 54. Thus, base 68 of float 40 can be slidably moved in an axial direction relative to portions of ballast 38 adjacent bottom end 54 thereof.

Separator 16 is assembled by resiliently engaging ballast mounting section 50 of bellows 36 with flange 56 of ballast 38. Float 40 then is urged upwardly through ballast 38 and into lower end 44 of bellows 36. After sufficient insertion, annular groove 64 of float 40 will engage annular bead 49 of bellows 36. Thus, bellows 36, ballast 38, and float 40 will be securely engaged with one another.

Portions of separator 16 adjacent upper end 42 of bellows 36 then are urged into recess 30 in bottom end 26 of closure 14. This insertion will cause arcuate flanges 34 of closure 14 to deflect. After sufficient insertion, arcuate flanges 34 will resiliently return toward an undeflected condition in which flanges 34 engage neck 48 of bellows 36. Additionally, the concave cone at upper end 42 of bellows 36 is deflected downwardly and into a convex shape by cone 32 of closure 14.

The subassembly comprised of closure 14 and separator 16 then is inserted into open top 20 of tube 12 such that separator 16 and lower end 26 of closure 14 lie within tube 12, as shown in FIGS. 12 and 13. Closure 14 will sealingly engage against interior surface regions and top end 20 of tube 12. Additionally, toroidal section 48 of bellows 36 will sealingly engage against inner surface 23 of tube 12.

As shown in FIG. 13, a liquid sample is delivered to the tube by a needle that penetrates septum 28 of closure 14 and upper end 42 of bellows 36. For purposes of illustration only, the liquid sample is blood. Blood will flow through central opening 62 of float 40 and to bottom end 18 of tube 12. The needle then will be withdrawn from assembly 10. Upon removal of the needle septum 28, closure 14 will reseal itself. Upper end 42 of bellows 36 also will reclose itself in a manner that will render it substantially impervious to fluid flow.

As shown in FIG. 14, when assembly 10 is subjected to centrifugation or to an axial centrifugation force, the respective phases of the blood will begin to separate so that the more dense phase comprising red blood cells will be displaced toward the bottom end 18 of tube 12 and so that the less dense phase comprising serum or plasma will be displaced to a location immediately above the denser phase. Simultaneously, the centrifugal loads will urge ballast 38 toward bottom end 18 of tube 12 relative to float 40. This movement of ballast 38 will generate a longitudinal deformation of bellows 36. As a result, toroidal sealing section 48 will become longer and narrower and will be spaced concentrically inwardly from the inner surface 23 of sidewall 20 of tube 12. The smaller cross-section of toroidal section 48 will permit a movement of portions of bellows 36 adjacent lower end 44 to move toward bottom 18 of tube 12. Upper end 42 of bellows 36 initially will be retained adjacent closure 14 by arcuate flanges 34. However, all of closure 14 is resiliently deformable, and hence arcuate flanges 34 will resiliently deform downwardly in response to centrifugal loads created on separator 16, and particularly on ballast 38. Hence, separator 16 will separate from closure 14 and will begin moving in tube 12 toward bottom end 18, as shown in FIG. 14. Air in portions of tube 12 between the blood and separator 16 will flow around separator 16 and into sections of tube 12 between separator 16 and closure 14. After

sufficient movement of separator 16, bottom end 54 of ballast 38 and/or bottom end 60 of float 40 will contact the top surface of the blood. This will leave trapped air within aperture 62 of float 40 that could impede further downward movement of separator 16. However, the defect in top 42 of bellows 36 caused by the needle cannula will enable trapped air to escape to regions of tube 12 between separator 16 and closure 14. Thus, ballast 38 will continue to urge separator 16 down into the separating blood with a liquid phase capable of moving around and above the separator. As noted above, separator 16 has an overall density between the densities of the formed and liquid phases of the blood. Consequently, separator 16 will stabilize in a position within tube 12 such that the formed phase of the blood will lie between bottom end 18 of tube 12 and separator 16, as shown in FIG. 15. The liquid phases of the blood will lie between separator 16 and closure 14.

After this stabilized state has been reached, the centrifuge will be stopped. The termination of the centrifugal load will cause toroidal sealing section 48 of bellows 36 to resiliently return toward its unbiased condition and into sealing engagement with interior surface 23 of tube 12. Thus, the formed and liquid phases of blood will be separated efficiently and can be accessed separately for analysis.

An alternate embodiment of the tube assembly in accordance with the subject invention is identified generally by the numeral 110 in FIG. 16. Assembly 110 includes a tube 112, a closure 114, and a separator 116.

Tube 112 includes an open top 118, a bottom 120, and a cylindrical wall 122 extending therebetween. Bottom 120 of tube 112 has an opening 124 extending therethrough. A bottom closure 126 is sealingly engaged in opening 124. Bottom closure 126 is formed from a needle pierceable elastomer and enables the formed phase of a blood sample to be accessed directly from bottom 120 of tube 112.

Closure 114 includes an elastomeric stopper 128 sealingly engaged in open top 118 of tube 112. Stopper 128 is provided with a centrally disposed needle pierceable septum 130. Stopper 128 further includes a bottom recess 132 having a plurality of inwardly directed resiliently deflectable arcuate flanges 134 extending thereabout.

Closure 114 further includes an outer cap 136 having an annular top wall 138 and a generally cylindrical skirt 140 depending downwardly from top wall 138. Cap 136 is securely mounted around stopper 128 and is removably mountable over open top 118 of tube 112. Top wall 138 of cap 136 is provided with a central opening 142 that substantially registers with septum 130.

Separator 116 includes a bellows 144, a ballast 146, and a float 148. Bellows 144 includes an upper end 150, a lower end 152, and a toroidal sealing 154 therebetween. Unlike the prior embodiment, portions of bellows 144 adjacent upper end 150 are not conically generated. Rather, these upper portions of bellows 144 are substantially spherically generated and will nest with recess 132 in stopper 128 without the inward deformation that had been described with respect to the first embodiment. Portions of bellows 144 adjacent lower end 152 and adjacent toroidal sealing 154 are substantially the same as in the prior embodiment.

Ballast 146 includes an upper end 156 and a lower end 158. Portions of ballast 146 in proximity to lower end 158 differ from the prior embodiment in that inwardly directed flanges 160 are provided for trapping float 148. Thus, any post-assembly downward movement of float 148 relative to ballast 146 is substantially prevented. However, upward movement of float 148 relative to ballast 146 is possible, and will occur during centrifugation.

Alternatively, it is possible for the separator element to be a unitary structure having regions of varying densities that provide the functionality of the buoyancy member and ballast member.

In one such embodiment, reflected in FIG. 17, the separator element **200** is a unitary element formed from a polymeric material, where the upper region **202** of the element comprises a lower-density material, and the lower region **204** contains a higher density material. Upon centrifugation, the lower and higher density regions would act as the buoyancy and ballast members, respectively. The middle region is not required to contribute to buoyancy or ballast, and may be equivalent to the overall density of the device. The separator element **200** may be spherical in shape, but variations are possible to optimize the sealing and movement of the separator for its intended application.

There are numerous molding techniques for fabricating such a separator. The equations and relationships disclosed herein can be used to determine a desired density distribution, and the various molding processes available can be adjusted accordingly.

In one technique, it is possible to mold a body from a single material, but with gas bubbles, either many small bubbles or one or a few large bubbles, dispersed in the upper region to provide a lowered density relative to the remainder of the separator. This could be done for example by use of a supercooled or supercritical fluid injected into the polymer material. One commercial technique for doing so is the MuCell® process owned by Trexel, Inc., Woburn, Mass., and reflected in U.S. Pat. Nos. 5,158,986, RE37,932, and 5,160,674, the disclosures of which are hereby incorporated by reference. Other conventional foaming techniques may also be used selectively during injection molding to provide a desired density.

In another technique, it is possible to add higher density additives to a lower region of a single material matrix, or to add lower density additives to an upper region of a single material matrix. For example, it is possible to perform injection molding with introduction of an additive (e.g., a low or high density additive) to provide a desired density gradient. As shown in the cross-section view of FIG. 18, this could be used to provide a separator **210** having a high density matrix **212** with low density additive **214** at an upper region thereof. This approach could also provide a low density matrix with high density components at a lower region thereof, or a matrix with high density additives at one region and low density additives at another region. The matrix may have a concentration gradient of the additive to provide a desirable density distribution, or may have isolated regions with additive present therein. Examples of suitable additives include solid or hollow beads such as glass beads, as well as hollow or solid fibers, and clay composites.

The separator may also be formed from two or more materials, e.g., compatible materials having different densities, by a technique such as two-shot molding (which can be more than two shots), or by co-injection molding. The separator may also be formed from the same material with differing molding parameters to provide differing densities, for example selective use of a process such as MuCell® or other selective incorporation of the additives noted above, or selective use of molding temperatures. Other processes that may be suitable include gas-assist, overmolding, and co-injection plus MuCell®.

The unitary separator is formed of any suitable materials that provide the needed density and elastomeric properties, are capable of being used with the techniques needed to form the unitary separator, and that are inert with respect to the

collected sample. One suitable material would be the Kraton™ family of materials (block copolymers of styrene and rubber); soft silicones are also possible.

As discussed above, it is generally desirable to direct blood into the container such that the blood is able to get beneath the separator, since serum tubes for some applications require the red blood cells to be below the separator (e.g., where the red blood cells clot and are to be separated from the serum). (This is less important for plasma tubes.) Such an outcome is difficult if the separator starts on the bottom of the tube. There are at least two solutions to this problem. One is to design the separator to be secured at the top of the blood collection tube, such that the non-patient end of the needle can be inserted through the separator into the tube interior. The separator would thus be formed of a material pierceable by such a needle, and of a size/shape to allow the needle to pass completely through. The shape of the separator would be designed accordingly, and thus might incorporate for example a divot or recess at its lower end to allow access through the separator into the reservoir portion of the tube. Securement of the separator at the top end of the tube could be attained by molding in a feature that mates with a corresponding feature of the tube closure, or by utilizing a tube taper that holds the separator at the top of the tube prior to centrifugation.

An alternative is to form a tube with openings (and stoppers) on both ends. The separator is inserted proximate the stopper at one end, and the blood is directed into the tube via the opposite stopper. For plasma separation tubes where an anticoagulant is present, the separator can be placed at the bottom of the tube initially, and blood can be directed onto it, without detrimental effects.

The separator would function essentially in the same manner as the multi-component separator discussed above. Specifically, upon centrifugation and immersion of the separator in the fluid, as reflected by the arrows A and B in FIG. 17, the lower density upper region **202** provides a buoyant upward force on the separator relative to the fluid. Simultaneously, the higher density lower region **204** provides an axial force downward on the separator. The combined forces stretch and elongate a middle region **203** of the separator axially, shown by arrows C, causing inward radial movement of the middle region. This radial movement pulls the separator out of contact with the inner wall of the tube so that it is free to move axially without any frictional drag. (Note that the middle region may have the same density as the upper or the lower region, but provides the sealing function due to its location in the middle portion of the separator.)

Therefore, a path is developed between the inner wall of the tube and the separator that permits the flow of the low-density blood component past the separator as it migrates down the tube. Migration of the separator terminates when it reaches the position between the lower density fluid component and higher density fluid or cellular/solid components, equal to its overall density. Upon terminating centrifugation, the separator expands to its undeformed shape, sealing against the inner wall of the tube, thereby creating a barrier between the higher and lower density components of the sample fluid.

Other embodiments of the invention will be apparent from the disclosure herein.

What is claimed is:

1. A method for manufacturing a biological fluid collection container having therein a separator for separating components of a blood sample to be collected into a higher density phase and a lower density phase, the method comprising:

13

providing the biological fluid collection container;
forming the separator, the separator comprising a first
region having a first density, a second region having a
second density, and a connecting middle region extend-
ing between the first region and the second region,
wherein the first density is less than the second density,
the connecting middle region is adapted to deform upon
application of rotational force while maintaining con-
tact with both the first region and the second region,
and the first region and the connecting middle region
comprise a first material and the second region com-
prises a second material, the first material being dif-
ferent from the second material; and

placing the separator into the container.

2. The method of claim 1, wherein the forming step
further comprises forming the separator from the first mate-
rial and the second material within a mold.

3. The method of claim 2, further comprising providing
one or more additives in at least one of the first material and
the second material.

14

4. The method of claim 3, wherein the one or more
additives are selected from the group consisting of beads and
fibers.

5. The method of claim 4, wherein the one or more
additives comprise hollow glass beads.

6. The method of claim 2, further comprising providing
voids or bubbles in at least one of the first material and the
second material.

7. The method of claim 6, wherein the voids or bubbles
are provided by injecting a supercritical or supercooled fluid
into at least one of the first material and the second material.

8. The method of claim 2, further comprising injecting the
first material and the second material into the mold.

9. The method of claim 2, wherein the forming step
comprises at least one molding process selected from the
group consisting of two-shot, overmolding, and co-injection.

* * * * *