



US009788942B2

(12) **United States Patent**
Backus et al.

(10) **Patent No.:** **US 9,788,942 B2**
(45) **Date of Patent:** **Oct. 17, 2017**

(54) **PROSTHETIC HEART VALVE HAVING TUBULAR SEAL**

(71) Applicant: **BOSTON SCIENTIFIC SCIMED, INC.**, Maple Grove, MN (US)

(72) Inventors: **Andrew J. H. Backus**, Santa Cruz, CA (US); **Spencer C. Noe**, Santa Cruz, CA (US); **Christopher M. Miracle**, Walnut Creek, CA (US)

(73) Assignee: **Boston Scientific Scimed Inc.**, Maple Grove, MN (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1 day.

(21) Appl. No.: **15/007,979**

(22) Filed: **Jan. 27, 2016**

(65) **Prior Publication Data**

US 2016/0220365 A1 Aug. 4, 2016

Related U.S. Application Data

(60) Provisional application No. 62/111,472, filed on Feb. 3, 2015.

(51) **Int. Cl.**
A61F 2/24 (2006.01)
A61F 2/90 (2013.01)

(52) **U.S. Cl.**
CPC *A61F 2/2418* (2013.01); *A61F 2/2415* (2013.01); *A61F 2/2436* (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC *A61F 2/24*; *A61F 2/2418*
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

51,922 A 6/1856 Peale
2,682,057 A 6/1954 Lord

(Continued)

FOREIGN PATENT DOCUMENTS

CN 1338951 A 3/2002
DE 19532846 A1 3/1997

(Continued)

OTHER PUBLICATIONS

US 8,062,356, 11/2011, Salahieh et al. (withdrawn)

(Continued)



Primary Examiner — Suzette J Gherbi

(74) *Attorney, Agent, or Firm* — Seager, Tufte & Wickhem, LLP

(57) **ABSTRACT**

A prosthetic heart valve includes a plurality of leaflets and an expandable member including one or more braided wires with a first set of wire segments extended helically in a first direction and a second set of wire segments extended helically in a second direction such that each wire segment of the first set intersects a plurality of wire segments from the second set at a plurality of intersection points. The one or more braided wires can have crowns where the wire segments of the first set connect to wire segments of the second set. The heart valve can include a tubular seal secured to the plurality of leaflets and to the expandable member by a plurality of sutures. The sutures can include cross stitches formed around both a wire segment of the first set and a wire segment of the second set at one of the intersection points.

19 Claims, 18 Drawing Sheets

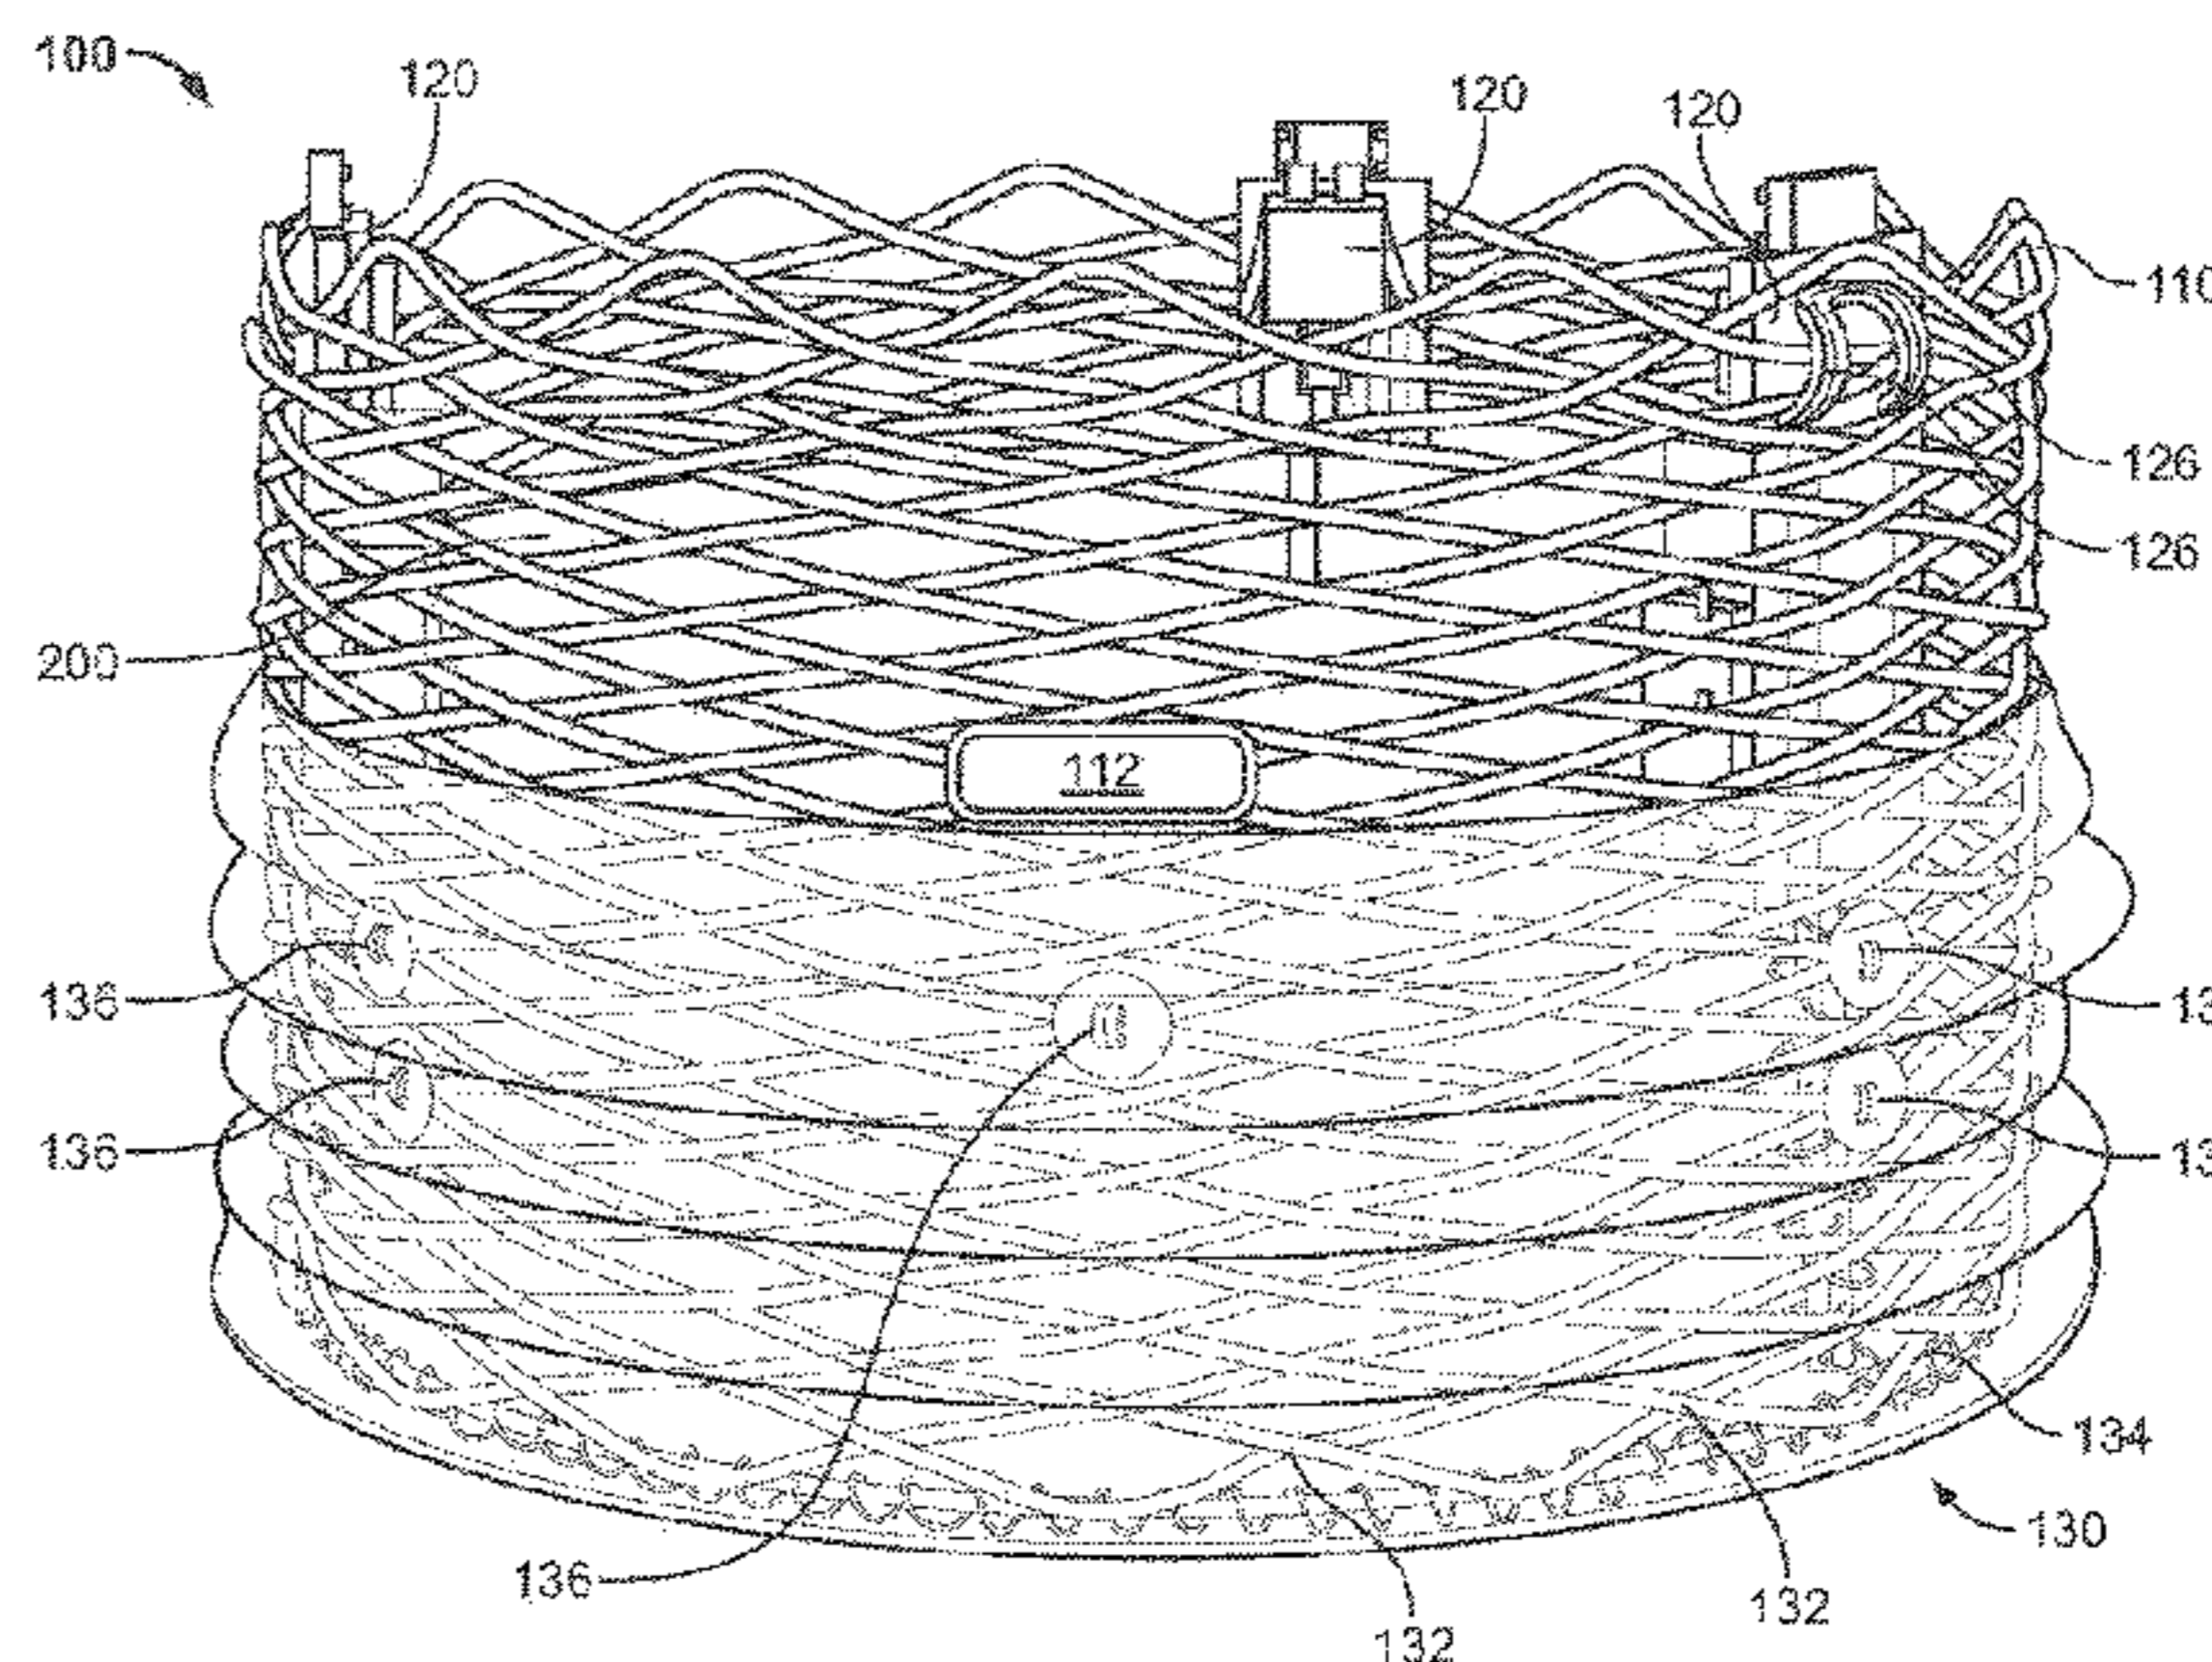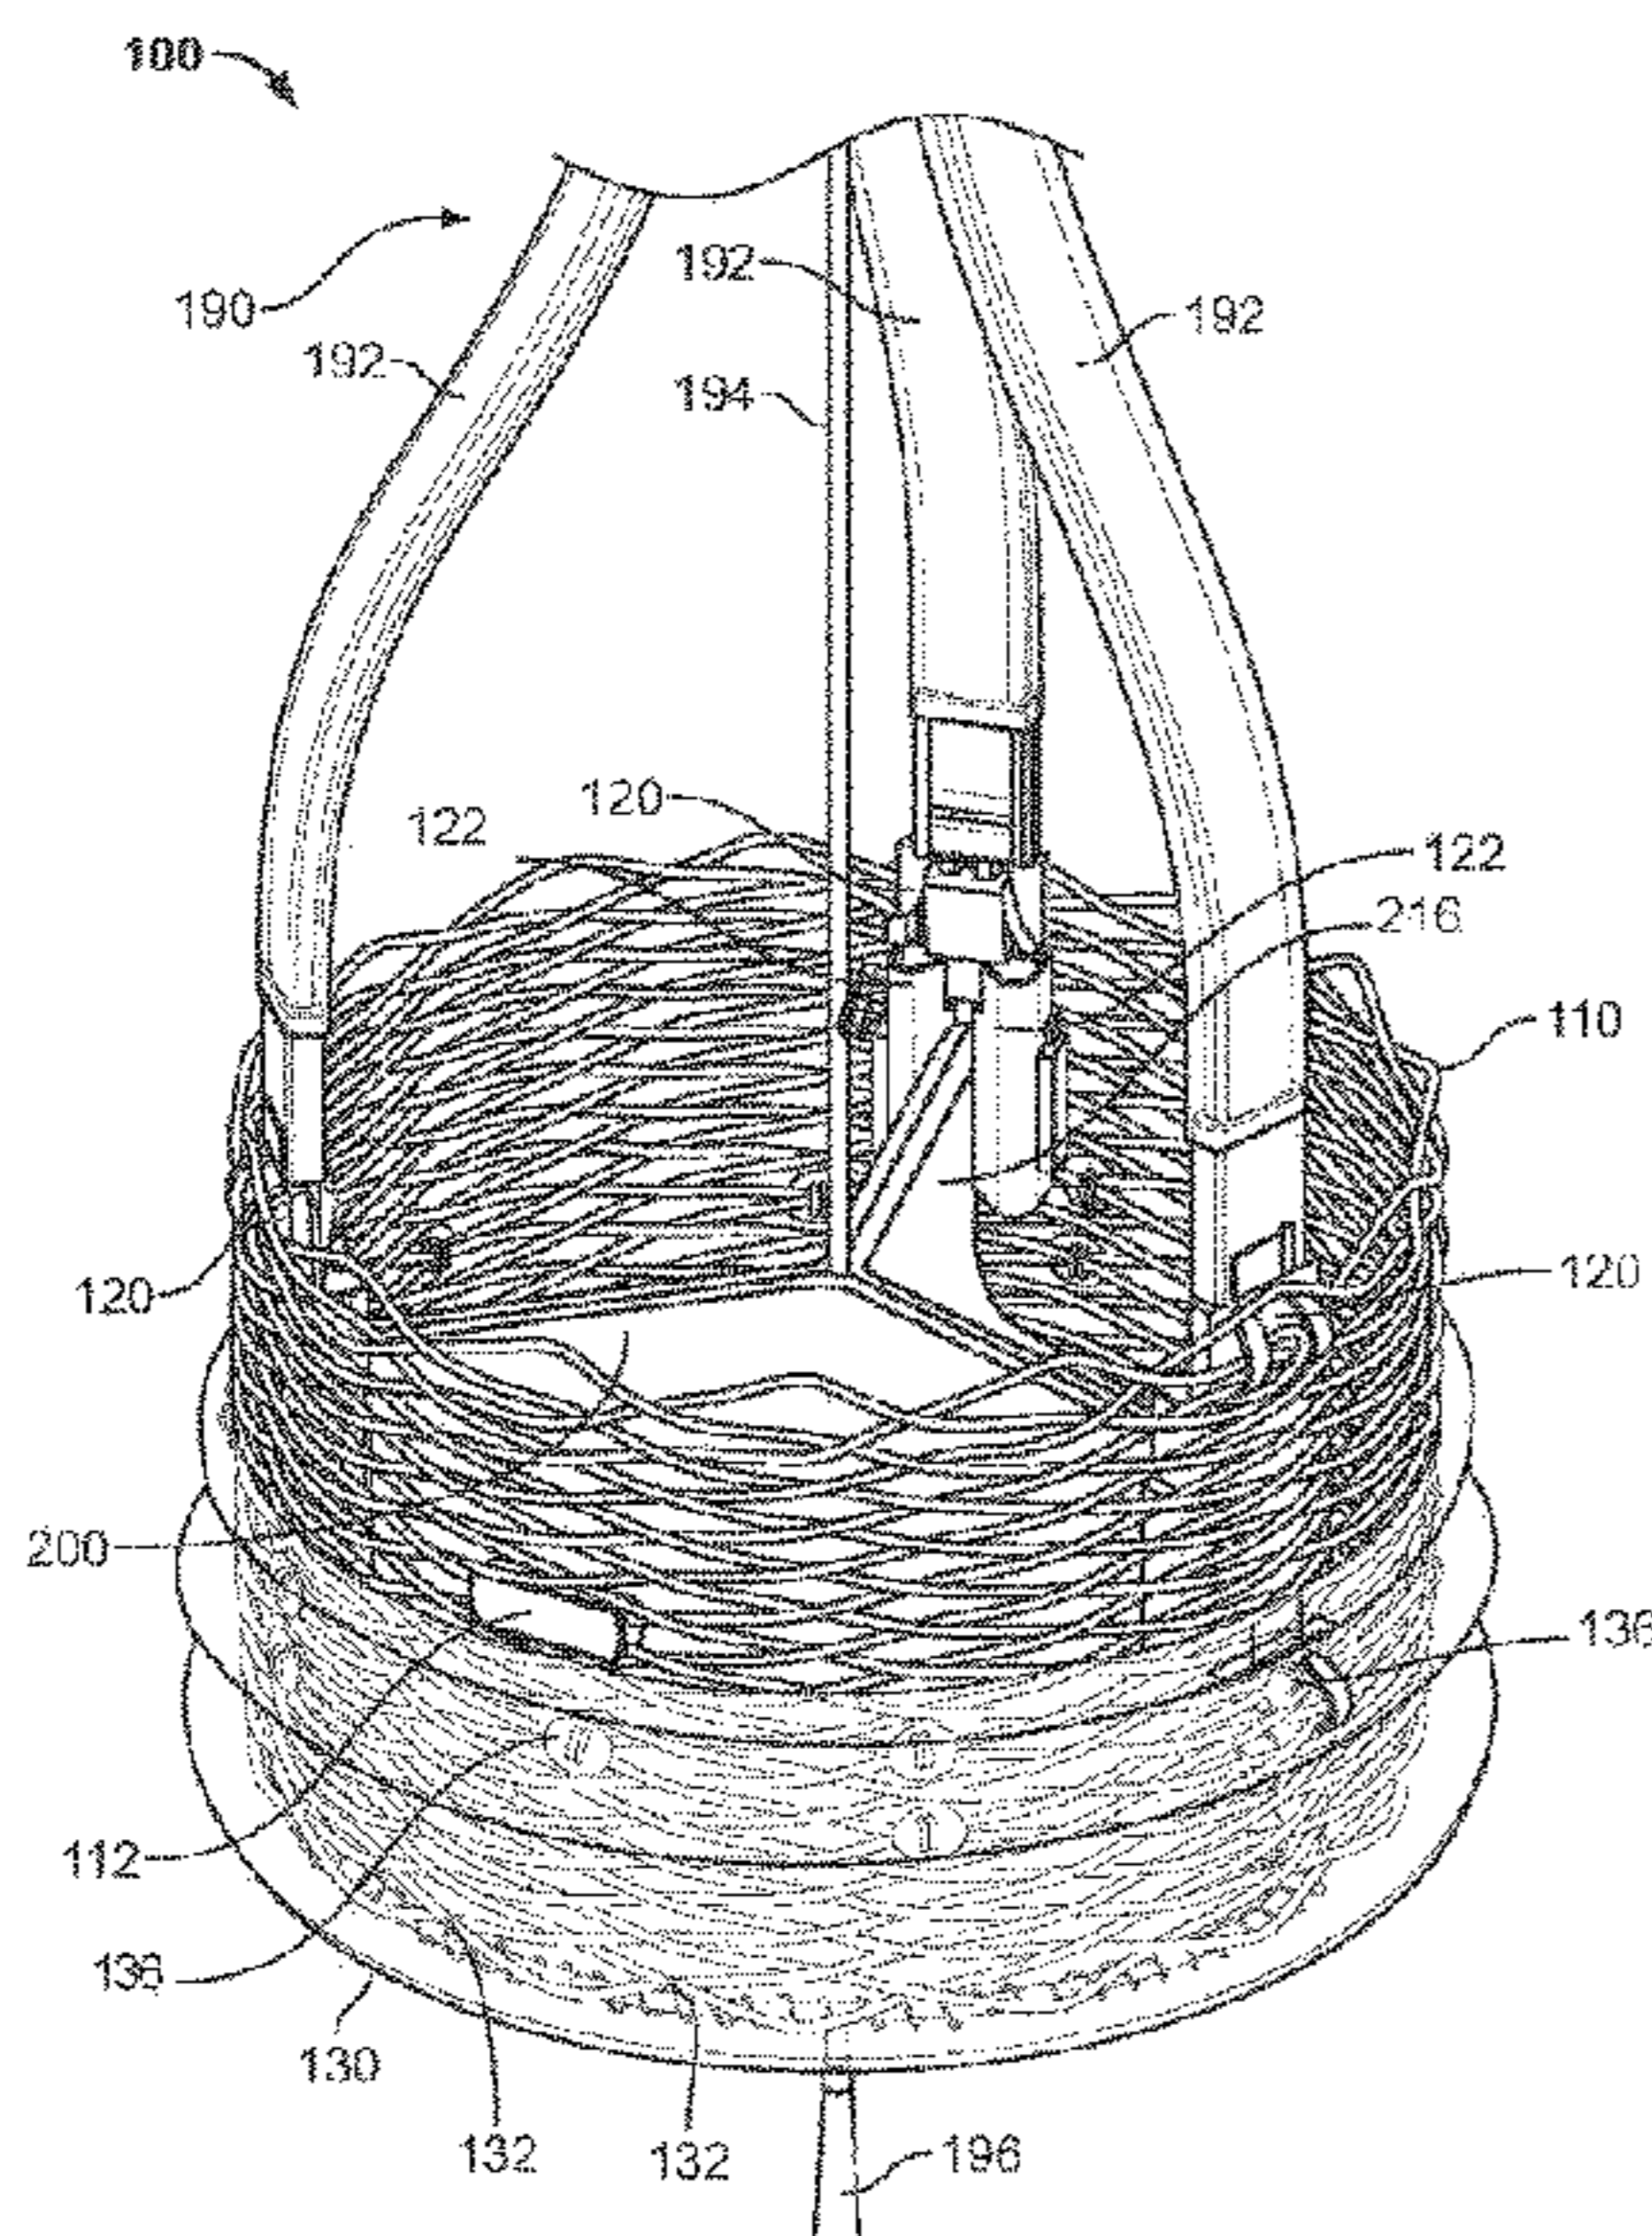

- (52) **U.S. Cl.**
 CPC *A61F 2/90* (2013.01); *A61F 2210/0057*
 (2013.01); *A61F 2220/0075* (2013.01); *A61F*
2250/0069 (2013.01)
- (58) **Field of Classification Search**
 USPC 623/1.15–1.53
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,701,559 A	2/1955	Cooper	4,710,192 A	12/1987	Liotta et al.
2,832,078 A	4/1958	Williams	4,733,665 A	3/1988	Palmaz
3,099,016 A	7/1963	Edwards	4,755,181 A	7/1988	Igoe
3,113,586 A	12/1963	Edmark, Jr.	4,759,758 A	7/1988	Gabbay
3,130,418 A	4/1964	Head et al.	4,777,951 A	10/1988	Cribier et al.
3,143,742 A	8/1964	Cromie	4,787,899 A	11/1988	Lazarus
3,334,629 A	8/1967	Cohn	4,787,901 A	11/1988	Baykut
3,367,364 A	2/1968	Cruz, Jr. et al.	4,796,629 A	1/1989	Grayzel
3,409,013 A	11/1968	Berry	4,819,751 A	4/1989	Shimada et al.
3,445,916 A	5/1969	Schulte	4,829,990 A	5/1989	Thuroff et al.
3,540,431 A	11/1970	Mobin-Uddin	4,834,755 A	5/1989	Silvestrini et al.
3,548,417 A	12/1970	Kischer et al.	4,851,001 A	7/1989	Taheri
3,570,014 A	3/1971	Hancock	4,856,516 A	8/1989	Hillstead
3,587,115 A	6/1971	Shiley	4,865,600 A	9/1989	Carpentier et al.
3,592,184 A	7/1971	Watkins et al.	4,872,874 A	10/1989	Taheri
3,628,535 A	12/1971	Ostrowsky et al.	4,873,978 A	10/1989	Ginsburg
3,642,004 A	2/1972	Osthagen et al.	4,878,495 A	11/1989	Grayzel
3,657,744 A	4/1972	Ersek	4,878,906 A	11/1989	Lindemann et al.
3,671,979 A	6/1972	Moulopoulos	4,883,458 A	11/1989	Shiber
3,714,671 A	2/1973	Edwards et al.	4,885,005 A	12/1989	Nashef et al.
3,755,823 A	9/1973	Hancock	4,909,252 A	3/1990	Goldberger
3,795,246 A	3/1974	Sturgeon	4,917,102 A	4/1990	Miller et al.
3,839,741 A	10/1974	Haller	4,922,905 A	5/1990	Strecker
3,868,956 A	3/1975	Alfidi et al.	4,927,426 A	5/1990	Dretler
3,874,388 A	4/1975	King et al.	4,954,126 A	9/1990	Wallsten
3,997,923 A	12/1976	Possis	4,966,604 A	10/1990	Reiss
4,035,849 A	7/1977	Angell et al.	4,969,890 A	11/1990	Sugita et al.
4,056,854 A	11/1977	Boretos et al.	4,979,939 A	12/1990	Shiber
4,106,129 A	8/1978	Carpentier et al.	4,986,830 A	1/1991	Owens et al.
4,222,126 A	9/1980	Boretos et al.	4,994,077 A	2/1991	Dobben
4,233,690 A	11/1980	Akins	5,002,556 A	3/1991	Ishida et al.
4,265,694 A	5/1981	Boretos et al.	5,002,559 A	3/1991	Tower
4,291,420 A	9/1981	Reul	5,007,896 A	4/1991	Shiber
4,297,749 A	11/1981	Davis et al.	5,026,366 A	6/1991	Leckrone
4,323,358 A	4/1982	Lentz et al.	5,032,128 A	7/1991	Alonso
4,326,306 A	4/1982	Poler	5,037,434 A	8/1991	Lane
4,339,831 A	7/1982	Johnson	5,047,041 A	9/1991	Samuels
4,343,048 A	8/1982	Ross et al.	5,064,435 A	11/1991	Porter
4,345,340 A	8/1982	Rosen	5,080,668 A	1/1992	Bolz et al.
4,373,216 A	2/1983	Klawitter	5,085,635 A	2/1992	Cragg
4,406,022 A	9/1983	Roy	5,089,015 A	2/1992	Ross
4,423,809 A	1/1984	Mazzocco	5,132,473 A	7/1992	Furutaka et al.
4,425,908 A	1/1984	Simon	5,141,494 A	8/1992	Danforth et al.
4,470,157 A	9/1984	Love	5,152,771 A	10/1992	Sabbaghian et al.
4,484,579 A	11/1984	Meno et al.	5,159,937 A	11/1992	Tremulis
4,501,030 A	2/1985	Lane	5,161,547 A	11/1992	Tower
4,531,943 A	7/1985	Van Tassel et al.	5,163,953 A	11/1992	Vince
4,535,483 A	8/1985	Klawitter et al.	5,167,628 A	12/1992	Boyles
4,574,803 A	3/1986	Storz	5,209,741 A	5/1993	Spaeth
4,580,568 A	4/1986	Gianturco	5,215,541 A	6/1993	Nashef et al.
4,592,340 A	6/1986	Boyles	5,217,483 A	6/1993	Tower
4,602,911 A	7/1986	Ahmadi et al.	5,238,004 A	8/1993	Sahatjian et al.
4,605,407 A	8/1986	Black et al.	5,258,023 A	11/1993	Reger
4,610,688 A	9/1986	Silvestrini et al.	5,258,042 A	11/1993	Mehta
4,612,011 A	9/1986	Kautzky	5,282,847 A	2/1994	Trescony et al.
4,617,932 A	10/1986	Kornberg	5,295,958 A	3/1994	Shturman
4,643,732 A	2/1987	Pietsch et al.	5,332,402 A	7/1994	Teitelbaum
4,647,283 A	3/1987	Carpentier et al.	5,336,258 A	8/1994	Quintero et al.
4,648,881 A	3/1987	Carpentier et al.	5,350,398 A	9/1994	Pavcnik et al.
4,655,218 A	4/1987	Kulik et al.	5,360,444 A	11/1994	Kusuhara
4,655,771 A	4/1987	Wallsten	5,370,685 A	12/1994	Stevens
4,662,885 A	5/1987	Dipisa, Jr.	5,389,106 A	2/1995	Tower
4,665,906 A	5/1987	Jervis	5,397,351 A	3/1995	Pavcnik et al.
4,680,031 A	7/1987	Alonso	5,409,019 A	4/1995	Wilk
4,692,164 A	9/1987	Dzemeshevich et al.	5,411,552 A	5/1995	Andersen et al.
4,705,516 A	11/1987	Barone et al.	5,425,762 A	6/1995	Muller
			5,431,676 A	7/1995	Dubrul et al.
			5,443,446 A	8/1995	Shturman
			5,443,449 A	8/1995	Buelna
			5,443,477 A	8/1995	Marin et al.
			5,443,495 A	8/1995	Buscemi et al.
			5,443,499 A	8/1995	Schmitt
			5,476,506 A	12/1995	Lunn
			5,476,510 A	12/1995	Eberhardt et al.
			5,480,423 A	1/1996	Ravenscroft et al.
			5,480,424 A	1/1996	Cox
			5,500,014 A	3/1996	Quijano et al.
			5,507,767 A	4/1996	Maeda et al.
			5,534,007 A	7/1996	St. Germain et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,545,133	A	8/1996	Burns et al.	6,022,370	A	2/2000	Tower
5,545,209	A	8/1996	Roberts et al.	6,027,520	A	2/2000	Tsugita et al.
5,545,211	A	8/1996	An et al.	6,027,525	A	2/2000	Suh et al.
5,545,214	A	8/1996	Stevens	6,042,598	A	3/2000	Tsugita et al.
5,549,665	A	8/1996	Vesely et al.	6,042,607	A	3/2000	Williamson, IV et al.
5,554,185	A	9/1996	Block et al.	6,051,014	A	4/2000	Jang
5,571,175	A	11/1996	Vanney et al.	6,059,827	A	5/2000	Fenton, Jr.
5,571,215	A	11/1996	Sterman et al.	6,074,418	A	6/2000	Buchanan et al.
5,573,520	A	11/1996	Schwartz et al.	6,093,203	A	7/2000	Uflacker
5,575,818	A	11/1996	Pinchuk	6,096,074	A	8/2000	Pedros
5,591,185	A	1/1997	Kilmer et al.	6,123,723	A	9/2000	Konya et al.
5,591,195	A	1/1997	Taheri et al.	6,132,473	A	10/2000	Williams et al.
5,607,464	A	3/1997	Trescony et al.	6,139,510	A	10/2000	Palermo
5,609,626	A	3/1997	Quijano et al.	6,142,987	A	11/2000	Tsugita
5,645,559	A	7/1997	Hachtman et al.	6,146,366	A	11/2000	Schachar
5,662,671	A	9/1997	Barbut et al.	6,162,245	A	12/2000	Jayaraman
5,667,523	A	9/1997	Bynon et al.	6,165,200	A	12/2000	Tsugita et al.
5,674,277	A	10/1997	Freitag	6,165,209	A	12/2000	Patterson et al.
5,693,083	A	12/1997	Baker et al.	6,168,579	B1	1/2001	Tsugita
5,693,310	A	12/1997	Gries et al.	6,168,614	B1	1/2001	Andersen et al.
5,695,498	A	12/1997	Tower	6,171,327	B1	1/2001	Daniel et al.
5,709,713	A	1/1998	Evans et al.	6,171,335	B1	1/2001	Wheatley et al.
5,713,951	A	2/1998	Garrison et al.	6,179,859	B1	1/2001	Bates et al.
5,713,953	A	2/1998	Vallana et al.	6,187,016	B1	2/2001	Hedges et al.
5,716,370	A	2/1998	Williamson, IV et al.	6,197,053	B1	3/2001	Cosgrove et al.
5,716,417	A	2/1998	Girard et al.	6,200,336	B1	3/2001	Pavcnik et al.
5,720,391	A	2/1998	Dohm et al.	6,214,036	B1	4/2001	Letendre et al.
5,725,549	A	3/1998	Lam	6,221,006	B1	4/2001	Dubrul et al.
5,728,068	A	3/1998	Leone et al.	6,221,091	B1	4/2001	Khosravi
5,733,325	A	3/1998	Robinson et al.	6,221,096	B1	4/2001	Aiba et al.
5,735,842	A	4/1998	Krueger et al.	6,221,100	B1	4/2001	Strecker
5,749,890	A	5/1998	Shaknovich	6,231,544	B1	5/2001	Tsugita et al.
5,755,783	A	5/1998	Stobie et al.	6,231,551	B1	5/2001	Barbut
5,756,476	A	5/1998	Epstein et al.	6,241,757	B1	6/2001	An et al.
5,769,812	A	6/1998	Stevens et al.	6,245,102	B1	6/2001	Jayaraman
5,772,609	A	6/1998	Nguyen et al.	6,251,135	B1	6/2001	Stinson et al.
5,800,456	A	9/1998	Maeda et al.	6,258,114	B1	7/2001	Konya et al.
5,800,531	A	9/1998	Cosgrove et al.	6,258,115	B1	7/2001	Dubrul
5,807,405	A	9/1998	Vanney et al.	6,258,120	B1	7/2001	McKenzie et al.
5,817,126	A	10/1998	Imran	6,258,129	B1	7/2001	Dybdal et al.
5,824,041	A	10/1998	Lenker et al.	6,267,783	B1	7/2001	Letendre et al.
5,824,043	A	10/1998	Cottone, Jr.	6,270,513	B1	8/2001	Tsugita et al.
5,824,053	A	10/1998	Khosravi et al.	6,277,555	B1	8/2001	Duran et al.
5,824,055	A	10/1998	Spiridigliozzi et al.	6,299,637	B1	10/2001	Shaolian et al.
5,824,056	A	10/1998	Rosenberg	6,302,906	B1	10/2001	Goicoechea et al.
5,824,064	A	10/1998	Taheri	6,309,417	B1	10/2001	Spence et al.
5,840,081	A	11/1998	Andersen et al.	6,319,281	B1	11/2001	Patel
5,843,158	A	12/1998	Lenker et al.	6,327,772	B1	12/2001	Zadno-Azizi et al.
5,855,597	A	1/1999	Jayaraman	6,336,934	B1	1/2002	Gilson et al.
5,855,601	A	1/1999	Bessler et al.	6,336,937	B1	1/2002	Vonesh et al.
5,855,602	A	1/1999	Angell	6,338,735	B1	1/2002	Stevens
5,860,966	A	1/1999	Tower	6,346,116	B1	2/2002	Brooks et al.
5,861,024	A	1/1999	Rashidi	6,348,063	B1	2/2002	Yassour et al.
5,861,028	A	1/1999	Angell	6,352,554	B2	3/2002	De Paulis
5,868,783	A	2/1999	Tower	6,352,708	B1	3/2002	Duran et al.
5,876,419	A	3/1999	Carpenter et al.	6,361,545	B1	3/2002	Macoviak et al.
5,876,448	A	3/1999	Thompson et al.	6,363,938	B2	4/2002	Saadat et al.
5,885,228	A	3/1999	Rosenman et al.	6,364,895	B1	4/2002	Greenhalgh
5,888,201	A	3/1999	Stinson et al.	6,371,970	B1	4/2002	Khosravi et al.
5,891,191	A	4/1999	Stinson	6,371,983	B1	4/2002	Lane
5,895,399	A	4/1999	Barbut et al.	6,379,383	B1	4/2002	Palmaz et al.
5,906,619	A	5/1999	Olson et al.	6,398,807	B1	6/2002	Chouinard et al.
5,907,893	A	6/1999	Zadno-Azizi et al.	6,402,736	B1	6/2002	Brown et al.
5,910,154	A	6/1999	Tsugita et al.	6,409,750	B1	6/2002	Hyodoh et al.
5,911,734	A	6/1999	Tsugita et al.	6,416,510	B1	7/2002	Altman et al.
5,925,063	A	7/1999	Khosravi	6,425,916	B1	7/2002	Garrison et al.
5,944,738	A	8/1999	Amplatz et al.	6,440,164	B1	8/2002	DiMatteo et al.
5,954,766	A	9/1999	Zadno-Azizi et al.	6,454,799	B1	9/2002	Schreck
5,957,949	A	9/1999	Leonhardt et al.	6,458,153	B1	10/2002	Bailey et al.
5,968,070	A	10/1999	Bley et al.	6,461,382	B1	10/2002	Cao
5,984,957	A	11/1999	Laptewicz, Jr. et al.	6,468,303	B1	10/2002	Amplatz et al.
5,984,959	A	11/1999	Robertson et al.	6,468,660	B2	10/2002	Ogle et al.
5,993,469	A	11/1999	McKenzie et al.	6,475,239	B1	11/2002	Campbell et al.
5,997,557	A	12/1999	Barbut et al.	6,482,228	B1	11/2002	Norred
6,010,522	A	1/2000	Barbut et al.	6,485,501	B1	11/2002	Green
				6,485,502	B2	11/2002	Don Michael et al.
				6,488,704	B1	12/2002	Connelly et al.
				6,494,909	B2	12/2002	Greenhalgh
				6,503,272	B2	1/2003	Duerig et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,508,803	B1	1/2003	Horikawa et al.	6,866,669	B2	3/2005	Buzzard et al.
6,508,833	B2	1/2003	Pavcnik et al.	6,872,223	B2	3/2005	Roberts et al.
6,527,800	B1	3/2003	McGuckin, Jr. et al.	6,872,226	B2	3/2005	Cali et al.
6,530,949	B2	3/2003	Konya et al.	6,875,231	B2	4/2005	Anduiza et al.
6,530,952	B2	3/2003	Vesely	6,881,220	B2	4/2005	Edwin et al.
6,537,297	B2	3/2003	Tsugita et al.	6,887,266	B2	5/2005	Williams et al.
6,540,768	B1	4/2003	Diaz et al.	6,890,340	B2	5/2005	Duane
6,562,058	B2	5/2003	Seguin et al.	6,893,459	B1	5/2005	Macoviak
6,569,196	B1	5/2003	Vesely	6,893,460	B2	5/2005	Spenser et al.
6,572,643	B1	6/2003	Gharibadeh	6,905,743	B1	6/2005	Chen et al.
6,585,766	B1	7/2003	Huynh et al.	6,908,481	B2	6/2005	Cribier
6,592,546	B1	7/2003	Barbut et al.	6,911,036	B2	6/2005	Douk et al.
6,592,614	B2	7/2003	Lenker et al.	6,911,043	B2	6/2005	Myers et al.
6,605,112	B1	8/2003	Moll et al.	6,936,058	B2	8/2005	Forde et al.
6,610,077	B1	8/2003	Hancock et al.	6,936,067	B2	8/2005	Buchanan
6,616,682	B2	9/2003	Joergensen et al.	6,939,352	B2	9/2005	Buzzard et al.
6,622,604	B1	9/2003	Chouinard et al.	6,951,571	B1	10/2005	Srivastava
6,623,518	B2	9/2003	Thompson et al.	6,953,332	B1	10/2005	Kurk et al.
6,623,521	B2	9/2003	Steinke et al.	6,964,673	B2	11/2005	Tsugita et al.
6,632,243	B1	10/2003	Zadno-Azizi et al.	6,969,395	B2	11/2005	Eskuri
6,635,068	B1	10/2003	Dubrul et al.	6,972,025	B2	12/2005	WasDyke
6,635,079	B2	10/2003	Unsworth et al.	6,974,464	B2	12/2005	Quijano et al.
6,652,571	B1	11/2003	White et al.	6,974,474	B2	12/2005	Pavcnik et al.
6,652,578	B2	11/2003	Bailey et al.	6,974,476	B2	12/2005	McGuckin, Jr. et al.
6,663,588	B2	12/2003	DuBois et al.	6,979,350	B2	12/2005	Moll et al.
6,663,663	B2	12/2003	Kim et al.	6,984,242	B2	1/2006	Campbell et al.
6,669,724	B2	12/2003	Park et al.	6,989,027	B2	1/2006	Allen et al.
6,673,089	B1	1/2004	Yassour et al.	7,004,176	B2	2/2006	Lau
6,673,109	B2	1/2004	Cox	7,011,681	B2	3/2006	Vesely
6,676,668	B2	1/2004	Mercereau et al.	7,018,406	B2	3/2006	Seguin et al.
6,676,692	B2	1/2004	Rabkin et al.	7,025,791	B2	4/2006	Levine et al.
6,676,698	B2	1/2004	McGuckin, Jr. et al.	7,037,331	B2	5/2006	Mitelberg et al.
6,682,543	B2	1/2004	Barbut et al.	7,041,132	B2	5/2006	Quijano et al.
6,682,558	B2	1/2004	Tu et al.	7,097,658	B2	8/2006	Oktay
6,682,559	B2	1/2004	Myers et al.	7,122,020	B2	10/2006	Mogul
6,685,739	B2	2/2004	DiMatteo et al.	7,125,418	B2	10/2006	Duran et al.
6,689,144	B2	2/2004	Gerberding	7,141,063	B2	11/2006	White et al.
6,689,164	B1	2/2004	Seguin	7,166,097	B2	1/2007	Barbut
6,692,512	B2	2/2004	Jang	7,175,653	B2	2/2007	Gaber
6,695,864	B2	2/2004	Macoviak et al.	7,175,654	B2	2/2007	Bonsignore et al.
6,695,865	B2	2/2004	Boyle et al.	7,175,656	B2	2/2007	Khairkhahan
6,702,851	B1	3/2004	Chinn et al.	7,189,258	B2	3/2007	Johnson et al.
6,712,842	B1	3/2004	Gifford, III et al.	7,191,018	B2	3/2007	Gielen et al.
6,712,843	B2	3/2004	Elliott	7,201,772	B2	4/2007	Schwammenthal et al.
6,714,842	B1	3/2004	Ito	7,235,093	B2	6/2007	Gregorich
6,719,789	B2	4/2004	Cox	7,258,696	B2	8/2007	Rabkin et al.
6,723,116	B2	4/2004	Taheri	7,267,686	B2	9/2007	DiMatteo et al.
6,730,118	B2	5/2004	Spenser et al.	7,276,078	B2	10/2007	Spenser et al.
6,730,377	B2	5/2004	Wang	7,322,932	B2	1/2008	Xie et al.
6,733,525	B2	5/2004	Yang et al.	7,326,236	B2	2/2008	Andreas et al.
6,736,846	B2	5/2004	Cox	7,329,279	B2	2/2008	Haug et al.
6,752,828	B2	6/2004	Thornton	7,374,560	B2	5/2008	Ressemann et al.
6,755,854	B2	6/2004	Gillick et al.	7,381,219	B2	6/2008	Salahieh et al.
6,758,855	B2	7/2004	Fulton, III et al.	7,381,220	B2	6/2008	Macoviak et al.
6,764,503	B1	7/2004	Ishimaru	7,399,315	B2	7/2008	Iobbi
6,764,509	B2	7/2004	Chinn et al.	7,445,631	B2	11/2008	Salahieh et al.
6,767,345	B2	7/2004	St. Germain et al.	7,470,285	B2	12/2008	Nugent et al.
6,769,434	B2	8/2004	Liddicoat et al.	7,491,232	B2	2/2009	Bolduc et al.
6,773,454	B2	8/2004	Wholey et al.	7,510,574	B2	3/2009	Lê et al.
6,776,791	B1	8/2004	Stallings et al.	7,524,330	B2	4/2009	Berrekouw
6,786,925	B1	9/2004	Schoon et al.	7,530,995	B2	5/2009	Quijano et al.
6,790,229	B1	9/2004	Berrekouw	7,544,206	B2	6/2009	Cohn
6,790,230	B2	9/2004	Beyersdorf et al.	7,622,276	B2	11/2009	Cunanan et al.
6,790,237	B2	9/2004	Stinson	7,628,803	B2	12/2009	Pavcnik et al.
6,792,979	B2	9/2004	Konya et al.	7,632,298	B2	12/2009	Hijlkema et al.
6,797,002	B2	9/2004	Spence et al.	7,674,282	B2	3/2010	Wu et al.
6,814,746	B2	11/2004	Thompson et al.	7,712,606	B2	5/2010	Salahieh et al.
6,821,297	B2	11/2004	Snyders	7,722,638	B2	5/2010	Deyette, Jr. et al.
6,830,585	B1	12/2004	Artorf et al.	7,722,662	B2	5/2010	Steinke et al.
6,837,901	B2	1/2005	Rabkin et al.	7,722,666	B2	5/2010	Lafontaine
6,840,957	B2	1/2005	DiMatteo et al.	7,736,388	B2	6/2010	Goldfarb et al.
6,843,802	B1	1/2005	Villalobos et al.	7,748,389	B2	7/2010	Salahieh et al.
6,849,085	B2	2/2005	Marton	7,758,625	B2	7/2010	Wu et al.
6,863,668	B2	3/2005	Gillespie et al.	7,780,725	B2	8/2010	Haug et al.
6,866,650	B2	3/2005	Stevens et al.	7,799,065	B2	9/2010	Pappas
				7,803,185	B2	9/2010	Gabbay
				7,824,442	B2	11/2010	Salahieh et al.
				7,824,443	B2	11/2010	Salahieh et al.
				7,833,262	B2	11/2010	McGuckin, Jr. et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,846,204 B2	12/2010	Letac et al.	2002/0177766 A1	11/2002	Mogul
7,892,292 B2	2/2011	Stack et al.	2002/0183781 A1	12/2002	Casey et al.
7,918,880 B2	4/2011	Austin	2002/0188341 A1	12/2002	Elliott
7,938,851 B2	5/2011	Olson et al.	2002/0188344 A1	12/2002	Bolea et al.
7,959,666 B2	6/2011	Salahieh et al.	2002/0193871 A1	12/2002	Beyersdorf et al.
7,959,672 B2	6/2011	Salahieh et al.	2003/0014104 A1	1/2003	Cribier
7,988,724 B2	8/2011	Salahieh et al.	2003/0023303 A1	1/2003	Palmaz et al.
8,048,153 B2	11/2011	Salahieh et al.	2003/0028247 A1	2/2003	Cali
8,052,749 B2	11/2011	Salahieh et al.	2003/0036791 A1	2/2003	Philipp et al.
8,136,659 B2	3/2012	Salahieh et al.	2003/0040736 A1	2/2003	Stevens et al.
8,157,853 B2	4/2012	Laske et al.	2003/0040771 A1	2/2003	Hyodoh et al.
8,182,528 B2	5/2012	Salahieh et al.	2003/0040772 A1	2/2003	Hyodoh et al.
8,192,351 B2	6/2012	Fishler et al.	2003/0040791 A1	2/2003	Oktay
8,226,710 B2	7/2012	Nguyen et al.	2003/0040792 A1	2/2003	Gabbay
8,231,670 B2	7/2012	Salahieh et al.	2003/0050694 A1	3/2003	Yang et al.
8,236,049 B2	8/2012	Rowe et al.	2003/0055495 A1	3/2003	Pease et al.
8,246,678 B2	8/2012	Salahieh et al.	2003/0057156 A1	3/2003	Peterson et al.
8,252,051 B2	8/2012	Chau et al.	2003/0060844 A1	3/2003	Borillo et al.
8,252,052 B2	8/2012	Salahieh et al.	2003/0069492 A1	4/2003	Abrams et al.
8,287,584 B2	10/2012	Salahieh et al.	2003/0069646 A1	4/2003	Stinson
8,308,798 B2	11/2012	Pintor et al.	2003/0070944 A1	4/2003	Nigam
8,323,335 B2	12/2012	Rowe et al.	2003/0100918 A1	5/2003	Duane
8,328,868 B2	12/2012	Paul et al.	2003/0100919 A1	5/2003	Hopkins et al.
8,343,213 B2	1/2013	Salahieh et al.	2003/0109924 A1	6/2003	Cribier
8,376,865 B2	2/2013	Forster et al.	2003/0109930 A1	6/2003	Bluni et al.
8,377,117 B2	2/2013	Keidar et al.	2003/0114912 A1	6/2003	Sequin et al.
8,398,708 B2	3/2013	Meiri et al.	2003/0114913 A1	6/2003	Spenser et al.
8,579,962 B2	11/2013	Salahieh et al.	2003/0125795 A1	7/2003	Pavcnik et al.
8,603,160 B2	12/2013	Salahieh et al.	2003/0130729 A1	7/2003	Paniagua et al.
8,617,236 B2	12/2013	Paul et al.	2003/0135257 A1	7/2003	Taheri
8,623,074 B2	1/2014	Ryan	2003/0144732 A1	7/2003	Cosgrove et al.
8,623,076 B2	1/2014	Salahieh et al.	2003/0149475 A1	8/2003	Hyodoh et al.
8,623,078 B2	1/2014	Salahieh et al.	2003/0149476 A1	8/2003	Damm et al.
8,668,733 B2	3/2014	Haug et al.	2003/0149478 A1	8/2003	Figulla et al.
8,828,078 B2	9/2014	Salahieh et al.	2003/0153974 A1	8/2003	Spenser et al.
8,840,662 B2	9/2014	Salahieh et al.	2003/0171803 A1	9/2003	Shimon
8,840,663 B2	9/2014	Salahieh et al.	2003/0176884 A1	9/2003	Berrada et al.
8,858,620 B2	10/2014	Salahieh et al.	2003/0181850 A1	9/2003	Diamond et al.
2001/0002445 A1	5/2001	Vesely	2003/0187495 A1	10/2003	Cully et al.
2001/0007956 A1	7/2001	Letac et al.	2003/0191516 A1	10/2003	Weldon et al.
2001/0010017 A1	7/2001	Letac et al.	2003/0195609 A1	10/2003	Berenstein et al.
2001/0021872 A1	9/2001	Bailey et al.	2003/0199759 A1	10/2003	Richard
2001/0025196 A1	9/2001	Chinn et al.	2003/0199913 A1	10/2003	Dubrul et al.
2001/0032013 A1	10/2001	Marton	2003/0199971 A1	10/2003	Tower et al.
2001/0039450 A1	11/2001	Pavcnik et al.	2003/0199972 A1	10/2003	Zadno-Azizi et al.
2001/0041928 A1	11/2001	Pavcnik et al.	2003/0208224 A1	11/2003	Broome
2001/0041930 A1	11/2001	Globerman et al.	2003/0212429 A1	11/2003	Keegan et al.
2001/0044634 A1	11/2001	Don Michael et al.	2003/0212452 A1	11/2003	Zadno-Azizi et al.
2001/0044652 A1	11/2001	Moore	2003/0212454 A1	11/2003	Scott et al.
2001/0044656 A1	11/2001	Williamson, IV et al.	2003/0216774 A1	11/2003	Larson
2002/0002396 A1	1/2002	Fulkerson	2003/0225445 A1	12/2003	Derus et al.
2002/0010489 A1	1/2002	Grayzel et al.	2003/0229390 A1	12/2003	Ashton et al.
2002/0026233 A1	2/2002	Shaknovich	2003/0233117 A1	12/2003	Adams et al.
2002/0029014 A1	3/2002	Jayaraman	2004/0019374 A1	1/2004	Hojeibane et al.
2002/0029981 A1	3/2002	Nigam	2004/0034411 A1	2/2004	Quijano et al.
2002/0032480 A1	3/2002	Spence et al.	2004/0039436 A1	2/2004	Spenser et al.
2002/0032481 A1	3/2002	Gabbay	2004/0049224 A1	3/2004	Buehlmann et al.
2002/0042651 A1	4/2002	Liddicoat et al.	2004/0049226 A1	3/2004	Keegan et al.
2002/0052651 A1	5/2002	Myers et al.	2004/0049262 A1	3/2004	Obermiller et al.
2002/0055767 A1	5/2002	Forde et al.	2004/0049266 A1	3/2004	Anduiza et al.
2002/0055769 A1	5/2002	Wang	2004/0059409 A1	3/2004	Stenzel
2002/0058995 A1	5/2002	Stevens	2004/0073198 A1	4/2004	Gilson et al.
2002/0077696 A1	6/2002	Zadno-Azizi et al.	2004/0082904 A1	4/2004	Houde et al.
2002/0082609 A1	6/2002	Green	2004/0082967 A1	4/2004	Broome et al.
2002/0095173 A1	7/2002	Mazzocchi et al.	2004/0087982 A1	5/2004	Eskuri
2002/0095209 A1	7/2002	Zadno-Azizi et al.	2004/0088045 A1	5/2004	Cox
2002/0111674 A1	8/2002	Chouinard et al.	2004/0093016 A1	5/2004	Root et al.
2002/0120328 A1	8/2002	Pathak et al.	2004/0093060 A1	5/2004	Seguin et al.
2002/0123802 A1	9/2002	Snyders	2004/0097788 A1	5/2004	Mourlas et al.
2002/0138138 A1	9/2002	Yang	2004/0098022 A1	5/2004	Barone
2002/0151970 A1	10/2002	Garrison et al.	2004/0098098 A1	5/2004	McGuckin, Jr. et al.
2002/0161390 A1	10/2002	Mouw	2004/0098099 A1	5/2004	McCullagh et al.
2002/0161392 A1	10/2002	Dubrul	2004/0098112 A1	5/2004	DiMatteo et al.
2002/0161394 A1	10/2002	Macoviak et al.	2004/0107004 A1	6/2004	Levine et al.
2002/0165576 A1	11/2002	Boyle et al.	2004/0111096 A1	6/2004	Tu et al.
			2004/0111146 A1	6/2004	McCullagh et al.
			2004/0116951 A1	6/2004	Rosengart
			2004/0117004 A1	6/2004	Osborne et al.
			2004/0117009 A1	6/2004	Cali et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2004/0122468	A1	6/2004	Yodfat et al.	2005/0137686	A1	6/2005	Salahieh et al.
2004/0122516	A1	6/2004	Fogarty et al.	2005/0137687	A1	6/2005	Salahieh et al.
2004/0127936	A1	7/2004	Salahieh et al.	2005/0137688	A1	6/2005	Salahieh et al.
2004/0127979	A1	7/2004	Wilson et al.	2005/0137689	A1	6/2005	Salahieh et al.
2004/0133274	A1	7/2004	Webler et al.	2005/0137690	A1	6/2005	Salahieh et al.
2004/0138694	A1	7/2004	Tran et al.	2005/0137691	A1	6/2005	Salahieh et al.
2004/0138742	A1	7/2004	Myers et al.	2005/0137692	A1	6/2005	Haug et al.
2004/0138743	A1	7/2004	Myers et al.	2005/0137693	A1	6/2005	Haug et al.
2004/0148018	A1	7/2004	Carpentier et al.	2005/0137694	A1	6/2005	Haug et al.
2004/0148021	A1	7/2004	Cartledge et al.	2005/0137695	A1	6/2005	Salahieh et al.
2004/0153094	A1	8/2004	Dunfee et al.	2005/0137696	A1	6/2005	Salahieh et al.
2004/0158277	A1	8/2004	Lowe et al.	2005/0137697	A1	6/2005	Salahieh et al.
2004/0167565	A1	8/2004	Beulke et al.	2005/0137698	A1	6/2005	Salahieh et al.
2004/0167620	A1	8/2004	Ortiz et al.	2005/0137699	A1	6/2005	Salahieh et al.
2004/0181140	A1	9/2004	Falwell et al.	2005/0137701	A1	6/2005	Salahieh et al.
2004/0186558	A1	9/2004	Pavcnik et al.	2005/0137702	A1	6/2005	Haug et al.
2004/0186563	A1	9/2004	Lobbi	2005/0143807	A1	6/2005	Pavcnik et al.
2004/0193261	A1	9/2004	Berrekouw	2005/0143809	A1	6/2005	Salahieh et al.
2004/0199245	A1	10/2004	Lauterjung	2005/0149159	A1	7/2005	Andreas et al.
2004/0204755	A1	10/2004	Robin	2005/0165352	A1	7/2005	Henry et al.
2004/0210304	A1	10/2004	Seguin et al.	2005/0165477	A1	7/2005	Anduiza et al.
2004/0210306	A1	10/2004	Quijano et al.	2005/0165479	A1	7/2005	Drews et al.
2004/0210307	A1	10/2004	Khairkhahan	2005/0182486	A1	8/2005	Gabbay
2004/0215331	A1	10/2004	Chew et al.	2005/0197694	A1	9/2005	Pai et al.
2004/0215333	A1	10/2004	Duran et al.	2005/0197695	A1	9/2005	Stacchino et al.
2004/0215339	A1	10/2004	Drasler et al.	2005/0203549	A1	9/2005	Realyvasquez
2004/0220655	A1	11/2004	Swanson et al.	2005/0203614	A1	9/2005	Forster et al.
2004/0225321	A1	11/2004	Krolik et al.	2005/0203615	A1	9/2005	Forster et al.
2004/0225352	A1*	11/2004	Osborne A61F 2/2418 623/1.24	2005/0203616	A1	9/2005	Cribier
2004/0225353	A1	11/2004	McGuckin, Jr. et al.	2005/0203617	A1	9/2005	Forster et al.
2004/0225354	A1	11/2004	Allen et al.	2005/0203618	A1	9/2005	Sharkawy et al.
2004/0225355	A1	11/2004	Stevens	2005/0209580	A1	9/2005	Freyman
2004/0243221	A1	12/2004	Fawzi et al.	2005/0228472	A1	10/2005	Case et al.
2004/0254636	A1	12/2004	Flagle et al.	2005/0228495	A1	10/2005	Macoviak
2004/0260390	A1	12/2004	Sarac et al.	2005/0234546	A1	10/2005	Nugent et al.
2005/0010287	A1	1/2005	Macoviak et al.	2005/0240200	A1	10/2005	Bergheim
2005/0021136	A1	1/2005	Xie et al.	2005/0240262	A1	10/2005	White
2005/0027348	A1*	2/2005	Case A61F 2/2412 623/1.24	2005/0251250	A1	11/2005	Verhoeven et al.
2005/0033398	A1	2/2005	Seguin	2005/0251251	A1	11/2005	Cribier
2005/0033402	A1	2/2005	Cully et al.	2005/0261759	A1	11/2005	Lambrecht et al.
2005/0043711	A1	2/2005	Corcoran et al.	2005/0267560	A1	12/2005	Bates
2005/0043757	A1	2/2005	Arad et al.	2005/0283231	A1	12/2005	Haug et al.
2005/0043790	A1	2/2005	Seguin	2005/0283962	A1	12/2005	Boudjemline
2005/0049692	A1	3/2005	Numamoto et al.	2006/0004439	A1	1/2006	Spenser et al.
2005/0049696	A1	3/2005	Siess et al.	2006/0004442	A1	1/2006	Spenser et al.
2005/0055088	A1	3/2005	Liddicoat et al.	2006/0015168	A1	1/2006	Gunderson
2005/0060016	A1	3/2005	Wu et al.	2006/0058872	A1	3/2006	Salahieh et al.
2005/0060029	A1	3/2005	Le et al.	2006/0149360	A1	7/2006	Schwammenthal et al.
2005/0065594	A1	3/2005	DiMatteo et al.	2006/0155312	A1	7/2006	Levine et al.
2005/0075584	A1	4/2005	Cali	2006/0161249	A1	7/2006	Realyvasquez et al.
2005/0075662	A1	4/2005	Pedersen et al.	2006/0173524	A1	8/2006	Salahieh et al.
2005/0075712	A1	4/2005	Biancucci et al.	2006/0195183	A1	8/2006	Navia et al.
2005/0075717	A1	4/2005	Nguyen et al.	2006/0253191	A1	11/2006	Salahieh et al.
2005/0075719	A1	4/2005	Bergheim	2006/0259134	A1	11/2006	Schwammenthal et al.
2005/0075724	A1	4/2005	Svanidze et al.	2006/0271166	A1	11/2006	Thill et al.
2005/0075730	A1	4/2005	Myers et al.	2006/0287668	A1	12/2006	Fawzi et al.
2005/0075731	A1	4/2005	Artof et al.	2006/0287717	A1	12/2006	Rowe et al.
2005/0085841	A1	4/2005	Eversull et al.	2007/0010876	A1	1/2007	Salahieh et al.
2005/0085842	A1	4/2005	Eversull et al.	2007/0010877	A1	1/2007	Salahieh et al.
2005/0085843	A1	4/2005	Opolski et al.	2007/0016286	A1	1/2007	Herrmann et al.
2005/0085890	A1	4/2005	Rasmussen et al.	2007/0055340	A1	3/2007	Pryor
2005/0090846	A1	4/2005	Pedersen et al.	2007/0061008	A1	3/2007	Salahieh et al.
2005/0090890	A1	4/2005	Wu et al.	2007/0112355	A1	5/2007	Salahieh et al.
2005/0096692	A1	5/2005	Linder et al.	2007/0118214	A1	5/2007	Salahieh et al.
2005/0096734	A1	5/2005	Majercak et al.	2007/0162107	A1	7/2007	Haug et al.
2005/0096735	A1	5/2005	Hojeibane et al.	2007/0173918	A1	7/2007	Dreher et al.
2005/0096736	A1	5/2005	Osse et al.	2007/0203503	A1	8/2007	Salahieh et al.
2005/0096738	A1	5/2005	Cali et al.	2007/0244552	A1	10/2007	Salahieh et al.
2005/0100580	A1	5/2005	Osborne et al.	2007/0288089	A1	12/2007	Gurskis et al.
2005/0107822	A1	5/2005	Wasdyke	2008/0009940	A1	1/2008	Cribier
2005/0113910	A1	5/2005	Paniagua et al.	2008/0033541	A1	2/2008	Gelbart et al.
2005/0131438	A1	6/2005	Cohn	2008/0082165	A1	4/2008	Wilson et al.
2005/0137683	A1	6/2005	Hezi-Yamit et al.	2008/0125859	A1	5/2008	Salahieh et al.
				2008/0188928	A1	8/2008	Salahieh et al.
				2008/0208328	A1	8/2008	Antocci et al.
				2008/0208332	A1	8/2008	Lamphere et al.
				2008/0221672	A1	9/2008	Lamphere et al.
				2008/0234814	A1	9/2008	Salahieh et al.
				2008/0255661	A1	10/2008	Straubinger et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0269878 A1 10/2008 Iobbi
 2008/0288054 A1 11/2008 Pulnev et al.
 2009/0005863 A1 1/2009 Goetz et al.
 2009/0030512 A1 1/2009 Thielen et al.
 2009/0054969 A1 2/2009 Salahieh et al.
 2009/0076598 A1 3/2009 Salahieh et al.
 2009/0093877 A1 4/2009 Keidar et al.
 2009/0171456 A1 7/2009 Kveen et al.
 2009/0222076 A1 9/2009 Figulla et al.
 2009/0264759 A1 10/2009 Byrd
 2009/0264997 A1 10/2009 Salahieh et al.
 2009/0299462 A1 12/2009 Fawzi et al.
 2010/0049313 A1 2/2010 Alon et al.
 2010/0094399 A1 4/2010 Dorn et al.
 2010/0121434 A1 5/2010 Paul et al.
 2010/0191326 A1 7/2010 Alkhatib
 2010/0219092 A1 9/2010 Salahieh et al.
 2010/0280495 A1 11/2010 Paul et al.
 2011/0257735 A1 10/2011 Salahieh et al.
 2011/0276122 A1* 11/2011 Schlick A61F 2/07
 623/1.13
 2011/0276129 A1 11/2011 Salahieh et al.
 2012/0016469 A1 1/2012 Salahieh et al.
 2012/0016471 A1 1/2012 Salahieh et al.
 2012/0022642 A1 1/2012 Haug et al.
 2012/0029627 A1 2/2012 Salahieh et al.
 2012/0041549 A1 2/2012 Salahieh et al.
 2012/0041550 A1 2/2012 Salahieh et al.
 2012/0046740 A1 2/2012 Paul et al.
 2012/0053683 A1 3/2012 Salahieh et al.
 2012/0089224 A1 4/2012 Haug et al.
 2012/0132547 A1 5/2012 Salahieh et al.
 2012/0197379 A1 8/2012 Laske et al.
 2012/0330409 A1 12/2012 Haug et al.
 2013/0013057 A1 1/2013 Salahieh et al.
 2013/0018457 A1 1/2013 Gregg et al.
 2013/0030520 A1 1/2013 Lee et al.
 2013/0123796 A1 5/2013 Sutton et al.
 2013/0158656 A1 6/2013 Sutton et al.
 2013/0190865 A1 7/2013 Anderson
 2013/0304199 A1 11/2013 Sutton et al.
 2014/0018911 A1 1/2014 Zhou et al.
 2014/0094904 A1 4/2014 Salahieh et al.
 2014/0114405 A1 4/2014 Paul et al.
 2014/0114406 A1 4/2014 Salahieh et al.
 2014/0121766 A1 5/2014 Salahieh et al.
 2014/0135912 A1 5/2014 Salahieh et al.
 2014/0243967 A1 8/2014 Salahieh et al.
 2014/0277417 A1 9/2014 Schraut et al.
 2015/0081000 A1* 3/2015 Hossainy A61F 2/88
 623/1.2
 2015/0134043 A1* 5/2015 Irwin A61F 2/88
 623/1.13
 2016/0256268 A1* 9/2016 Dakin A61B 17/12122
 2016/0296329 A1* 10/2016 Alkhatib A61F 2/2418

FOREIGN PATENT DOCUMENTS

DE 19546692 A1 6/1997
 DE 19857887 A1 7/2000
 DE 19907646 A1 8/2000
 DE 10049812 A1 4/2002
 DE 10049813 C1 4/2002
 DE 10049814 A1 4/2002
 DE 10049815 A1 4/2002
 EP 0103546 B1 5/1988
 EP 0144167 B1 11/1989
 EP 0409929 B1 4/1997
 EP 0850607 A1 7/1998
 EP 0597967 B1 12/1999
 EP 1000590 A1 5/2000
 EP 1057459 A1 12/2000
 EP 1057460 A1 12/2000
 EP 1088529 A2 4/2001

EP 0937439 B1 9/2003
 EP 1340473 A2 9/2003
 EP 1356793 A2 10/2003
 EP 1042045 B1 5/2004
 EP 0819013 B1 6/2004
 EP 1430853 A2 6/2004
 EP 1435879 A1 7/2004
 EP 1439800 A2 7/2004
 EP 1472996 A1 11/2004
 EP 1229864 B1 4/2005
 EP 1059894 B1 7/2005
 EP 1551274 A2 7/2005
 EP 1551336 A1 7/2005
 EP 1078610 B1 8/2005
 EP 1562515 A1 8/2005
 EP 1570809 A1 9/2005
 EP 1576937 A2 9/2005
 EP 1582178 A2 10/2005
 EP 1582179 A2 10/2005
 EP 1469797 B1 11/2005
 EP 1589902 A1 11/2005
 EP 1600121 A1 11/2005
 EP 1156757 B1 12/2005
 EP 1616531 A2 1/2006
 EP 1605871 B1 7/2008
 FR 2788217 A1 7/2000
 GB 2056023 A 3/1981
 GB 2398245 A 8/2004
 SU 1271508 A1 11/1986
 SU 1371700 A1 2/1988
 WO 9117720 A1 11/1991
 WO 9217118 A1 10/1992
 WO 9301768 A1 2/1993
 WO 9315693 A1 8/1993
 WO 9504556 A2 2/1995
 WO 9529640 A1 11/1995
 WO 9614032 A1 5/1996
 WO 9624306 A1 8/1996
 WO 9640012 A1 12/1996
 WO 9829057 A1 7/1998
 WO 9836790 A1 8/1998
 WO 9850103 A1 11/1998
 WO 9857599 A2 12/1998
 WO 9933414 A1 7/1999
 WO 9940964 A1 8/1999
 WO 9944542 A2 9/1999
 WO 9947075 A1 9/1999
 WO 9009059 A2 2/2000
 WO 0041652 A1 7/2000
 WO 0044308 A2 8/2000
 WO 0044311 A2 8/2000
 WO 0044313 A1 8/2000
 WO 0045874 A1 8/2000
 WO 0047139 A1 8/2000
 WO 0049970 A1 8/2000
 WO 0067661 A2 11/2000
 WO 0105331 A1 1/2001
 WO 0108596 A1 2/2001
 WO 0110320 A1 2/2001
 WO 0110343 A1 2/2001
 WO 0135870 A1 5/2001
 WO 0149213 A2 7/2001
 WO 0154625 A1 8/2001
 WO 0162189 A1 8/2001
 WO 0164137 A1 9/2001
 WO 0176510 A2 10/2001
 WO 0197715 A1 12/2001
 WO 0236048 A1 5/2002
 WO 0241789 A2 5/2002
 WO 0243620 A1 6/2002
 WO 0247575 A2 6/2002
 WO 02056955 A1 7/2002
 WO 02100297 A2 12/2002
 WO 03003943 A2 1/2003
 WO 03003949 A2 1/2003
 WO 03011195 A2 2/2003
 WO 03028592 A1 4/2003
 WO 03030776 A2 4/2003
 WO 03037227 A2 5/2003

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	03047648	A2	6/2003
WO	03015851	B1	11/2003
WO	03094793	A1	11/2003
WO	03094797	A1	11/2003
WO	2004006803	A1	1/2004
WO	2004006804	A1	1/2004
WO	2004014256	A1	2/2004
WO	2004019811	A2	3/2004
WO	2004019817	A1	3/2004
WO	2004021922	A2	3/2004
WO	2004023980	A2	3/2004
WO	2004026117	A2	4/2004
WO	2004041126	A1	5/2004
WO	2004043293	A2	5/2004
WO	2004047681	A1	6/2004
WO	2004058106	A2	7/2004
WO	2004066876	A1	8/2004
WO	2004082536	A1	9/2004
WO	2004089250	A1	10/2004
WO	2004089253	A1	10/2004
WO	2004093728	A2	11/2004
WO	2004105651	A1	12/2004
WO	2005002466	A2	1/2005
WO	2005004753	A1	1/2005
WO	2005009285	A2	2/2005
WO	2005011534	A1	2/2005
WO	2005011535	A2	2/2005
WO	2005023155	A1	3/2005
WO	2005027790	A1	3/2005
WO	2005046528	A1	5/2005
WO	2005046529	A1	5/2005
WO	2005048883	A1	6/2005
WO	2005062980	A2	7/2005
WO	2005065585	A1	7/2005
WO	2005084595	A1	9/2005
WO	2005087140	A1	9/2005
WO	2005096993	A1	10/2005
WO	2006005015	A2	1/2006
WO	2006009690	A1	1/2006
WO	2006027499	A2	3/2006
WO	2006138391	A2	12/2006
WO	2007033093	A2	3/2007
WO	2007035471	A2	3/2007
WO	2007044285	A2	4/2007
WO	2007053243	A2	5/2007
WO	2007058847	A2	5/2007
WO	2007092354	A2	8/2007
WO	2007097983	A2	8/2007
WO	2010042950	A2	4/2010
WO	2012116368	A2	8/2012

OTHER PUBLICATIONS

US 8,062,357, 11/2011, Salahieh et al. (withdrawn)

US 8,075,614, 12/2011, Salahieh et al. (withdrawn)

US 8,133,271, 03/2012, Salahieh et al. (withdrawn)

US 8,211,170, 07/2012, Paul et al. (withdrawn)

Andersen et al., "Transluminal implantation of artificial heart valves. Description of a new expandable aortic valve and initial results with implantation by catheter technique in closed chest pigs." *Euro. Heart J.*, 13:704-708, 1992.

Atwood et al., "Insertation of Heart Valves by Catheterization." Project Supervised by Prof. S. Muftu of Northeastern University 2001-2002: 36-40.

Bodnar et al., "Replacement Cardiac Valves R Chapter 13: Extinct Cardiac Valve Prostheses." Pergamon Publishing Corporation. New York, 1991: 307-322.

Boudjemline et al., "Percutaneous Implantation of a Biological Valve in the Aorta to Treat Aortic Valve Insufficiency—A Sheep Study." *Med Sci. Monit.*, vol. 8, No. 4: BR113-116, 2002.

Boudjemline et al., "Percutaneous Implantation of a Valve in the Descending Aorta in Lambs." *Euro. Heart J.*, 23: 1045-1049, 2002.

Boudjemline et al., "Percutaneous Pulmonary Valve Replacement in a Large Right Ventricular Outflow Tract: An Experimental Study." *Journal of the American College of Cardiology*, vol. 43(6): 1082-1087, 2004.

Boudjemline et al., "Percutaneous Valve Insertion: A New Approach?" *J. of Thoracic and Cardio. Surg.*, 125(3): 741-743, 2003.

Boudjemline et al., "Steps Toward Percutaneous Aortic Valve Replacement." *Circulation*, 105: 775-778, 2002.

Cribier et al., "Early Experience with Percutaneous Transcatheter Implantation of Heart Valve Prosthesis for the Treatment of End-Stage Inoperable Patients with Calcific Aortic Stenosis." *J. of Am. Coll. of Cardio*, 43(4): 698-703, 2004.

Cribier et al., "Percutaneous Transcatheter Implementation of an Aortic Valve Prosthesis for Calcific Aortic Stenosis: First Human Case Description." *Circulation*, 106: 3006-3008, 2002.

Cribier et al., "Percutaneous Transcatheter Implantation of an Aortic Valve Prosthesis for Calcific Aortic Stenosis: First Human Case." *Percutaneous Valve Technologies, Inc.*, 16 pages, 2002.

Ferrari et al., "Percutaneous Transvascular Aortic Valve Replacement with Self-Expanding Stent-Valve Device." Poster from the presentation given at SMIT 2000, 12th International Conference. Sep. 5, 2000.

Hijazi, "Transcatheter Valve Replacement: A New Era of Percutaneous Cardiac Intervention Begins." *J. of Am. College of Cardio.*, 43(6): 1088-1089, 2004.

Huber et al., "Do Valved Stents Compromise Coronary Flow?" *European Journal of Cardio-thoracic Surgery*, vol. 25: 754-759, 2004.

Knudsen et al., "Catheter-implanted prosthetic heart valves." *Int'l J. of Art. Organs*, 16(5): 253-262, 1993.

Kort et al., "Minimally Invasive Aortic Valve Replacement: Echocardiographic and Clinical Results." *Am. Heart J.*, 142(3): 476-481, 2001.

Love et al., "The Autogenous Tissue Heart Valve: Current Status." *Journal of Cardiac Surgery*, 6(4): 499-507, 1991.

Lutter et al., "Percutaneous Aortic Valve Replacement: An Experimental Study. I. Studies on Implantation." *J. of Thoracic and Cardio. Surg.*, 123(4): 768-776, 2002.

Moulopoulos et al., "Catheter-Mounted Aortic Valves." *Annals of Thoracic Surg.*, 11(5): 423-430, 1971.

Paniagua et al., "Percutaneous Heart Valve in the Chronic in Vitro Testing Model." *Circulation*, 106: e51-e52, 2002.

Paniagua et al., "Heart Watch." *Texas Heart Institute*. Spring, 2004. Edition: 8 pages.

Pavcnik et al., "Percutaneous Bioprosthetic Veno Valve: A Long-term Study in Sheep." *J. of Vascular Surg.*, 35(3): 598-603, 2002.

Phillips et al., "A Temporary Catheter-Tip Aortic Valve: Hemodynamic Effects on Experimental Acute Aortic Insufficiency." *Annals of Thoracic Surg.*, 21(2): 134-136, 1976.

Sochman et al., "Percutaneous Transcatheter Aortic Disc Valve Prosthesis Implantation: A Feasibility Study." *Cardiovasc. Intervent. Radiol.*, 23: 384-388, 2000.

Stuart, "In Heart Valves, A Brave, New Non-Surgical World." *Start-Up*. Sep. 17, 2004.

Vahanian et al., "Percutaneous Approaches to Valvular Disease." *Circulation*, 109: 1572-1579, 2004.

Van Herwerden et al., "Percutaneous Valve Implantation: Back to the Future?" *Euro. Heart J.*, 23(18): 1415-1416, 2002.

Zhou et al., "Self-expandable Valved Stent of Large Size: Off-Bypass Implantation in Pulmonary Position." *Eur. J. Cardiothorac.*, 24: 212-216, 2003.

Examiner's First Report on AU Patent Application No. 2011202667, issued on May 17, 2012.

"A Matter of Size." *Treennial Review of the National Nanotechnology Initiative*, The National Academies Press, Washington DC, v-13, 2006, <http://www.nap.edu/catalog/117521a-matter-of-size-treennial-review-of-the-national-nanotechnology>.

Atwood et al., "Insertion of Heart Valves by Catheterization." *The Capstone Design Course Report*. MIME 1501-1502. Technical Design Report. Northeastern University, pp. 1-93, Nov. 5, 2007.

Aug. 19, 2011, Supplemental Search Report from EP Patent Office, EP Application No. 04813777.2.

(56)

References Cited

OTHER PUBLICATIONS

Aug. 19, 2011, Supplemental Search Report from EP Patent Office, EP Application No. 04815634.3.

Cunanan et al., "Tissue Characterization and Calcification Potential of Commercial Bioprosthetic Heart Valves." *Ann. Thorac. Surg.*, S417-421, 2001.

Cunliffe et al., "Glutaraldehyde Inactivation of Exotic Animal Viruses in Swine Heart Tissue." *Applied and Environmental Microbiology*, Greenport, New York, 37(5): 1044-1046, May 1979.

EP Search Report mailed Aug. 10, 2011 for EP Application No. 06824992.9.

"Heart Valve Materials—Bovine (cow)." Equine & Porcine Pericardium, Maverick Biosciences Pty. Lt, <http://maverickbio.com/biological-medical-device-materials.php?htm>. 2009.

Helmus, "Mechanical and Bioprosthetic Heart Valves in Biomaterials for Artificial Organs." Woodhead Publishing Limited: 114-162, 2011.

Hourihan et al., "Transcatheter Umbrella Closure of Valvular and Paravalvular Leaks." *JACC*, Boston, Massachusetts, 20(6): 1371-1377, Nov. 15, 1992.

Laborde et al., "Percutaneous Implantation of the Corevalve Aortic Valve Prosthesis for Patients Presenting High Risk for Surgical Valve Replacement." *EuroIntervention*: 472-474, 2006.

Levy, "Mycobacterium Chelonae Infection of Porcine Heart Valves." *The New England Journal of Medicine*, Washington DC, 297(12), Sep. 22, 1977.

Supplemental Search Report from EP Patent Office, EP Application No. 05758878.2, Oct. 24, 2011.

"Pericardial Heart Valves." Edwards Lifesciences, Cardiovascular Surgery FAQ, Nov. 14, 2010, <http://www.edwards.com/products/cardiovascularsurgeryfaq.htm>.

Southern Lights Biomaterials Homepage, Jan. 7, 2011, <http://www.slv.co.nz/>.

Stassano. "Mid-term Results of the Valve-on-Valve Technique for Bioprosthetic Failure." *European Journal of Cardiothoracic Surgery*: 453-457, 2000.

Topol. "Percutaneous Expandable Prosthetic Valves." *Textbook of Interventional Cardiology*, W.B. Saunders Company, 2: 1268-1276, 1994.

Andersen et al., "Transluminal implantation of artificial heart valves. Description of a new expandable aortic valve and initial results with implantation by catheter technique in closed chest pigs." *Euro. Heart J.*, 13:704-708, May 1992.

Atwood et al., "Insertion of Heart Valves by Catheterization." Project Supervised by Prof. S. Muftu of Northeastern University 2001-2002: 36-40, May 30, 2002.

Bodnar et al., "Replacement Cardiac Valves R Chapter 13: Extinct Cardiac Valve Prostheses." Pergamon Publishing Corporation. New York, 307-322, 1991.

Boudjemline et al., "Percutaneous Implantation of a Biological Valve in the Aorta to Treat Aortic Valve Insufficiency—A Sheep Study." *Med Sci. Monit.*, vol. 8, No. 4: BR113-116, Apr. 12, 2002.

Boudjemline et al., "Percutaneous Implantation of a Valve in the Descending Aorta in Lambs." *Euro. Heart J.*, 23: 1045-1049, Jul. 2002.

Boudjemline et al., "Percutaneous Pulmonary Valve Replacement in a Large Right Ventricular Outflow Tract: An Experimental Study." *Journal of the American College of Cardiology*, vol. 43(6): 1082-1087, Mar. 17, 2004.

Boudjemline et al., "Percutaneous Valve Insertion: A New Approach?" *J. of Thoracic and Cardio. Surg.*, 125(3): 741-743, Mar. 2003.

Boudjemline et al., "Steps Toward Percutaneous Aortic Valve Replacement." *Circulation*, 105: 775-778, Feb. 12, 2002.

Cribier et al., "Early Experience with Percutaneous Transcatheter Implantation of Heart Valve Prosthesis for the Treatment of End-

Stage Inoperable Patients with Calcific Aortic Stenosis." *J. of Am. Coll. of Cardio*, 43(4): 698-703, Feb. 18, 2004.

Cribier et al., "Percutaneous Transcatheter Implementation of an Aortic Valve Prosthesis for Calcific Aortic Stenosis: First Human Case Description." *Circulation*, 106: 3006-3008, Dec. 10, 2002.

Cribier et al., "Percutaneous Transcatheter Implantation of an Aortic Valve Prosthesis for Calcific Aortic Stenosis: First Human Case." *Percutaneous Valve Technologies, Inc.*, 16 pages, Apr. 16, 2002.

Hijazi, "Transcatheter Valve Replacement: A New Era of Percutaneous Cardiac Intervention Begins." *J. of Am. College of Cardio.*, 43(6): 1088-1089, Mar. 17, 2004.

Huber et al., "Do Valved Stents Compromise Coronary Flow?" *European Journal of Cardio-thoracic Surgery*, vol. 25: 754-759, Jan. 23, 2004.

Knudsen et al., "Catheter-implanted prosthetic heart valves." *Int'l J. of Art. Organs*, 16(5): 253-262, May 1993.

Kort et al., "Minimally Invasive Aortic Valve Replacement: Echocardiographic and Clinical Results." *Am. Heart J.*, 142(3): 476-481, Sep. 2001.

Love et al., "The Autogenous Tissue Heart Valve: Current Status." *Journal of Cardiac Surgery*, 6(4): 499-507, Mar. 1991.

Lutter et al., "Percutaneous Aortic Valve Replacement: An Experimental Study. I. Studies on Implantation." *J. of Thoracic and Cardio. Surg.*, 123(4): 768-776, Apr. 2002.

Moulopoulos et al., "Catheter-Mounted Aortic Valves." *Annals of Thoracic Surg.*, 11(5): 423-430, May 1971.

Paniagua et al., "Percutaneous Heart Valve in the Chronic in Vitro Testing Model." *Circulation*, 106: e51-e52, Sep. 17, 2002.

Paniagua et al., "Heart Watch." Texas Heart Institute. Edition: 8 pages, Spring, 2004.

Pavcnik et al., "Percutaneous Bioprosthetic Venous Valve: A Long-term Study in Sheep." *J. of Vascular Surg.*, 35(3): 598-603, Mar. 2002.

Phillips et al., "A Temporary Catheter-Tip Aortic Valve: Hemodynamic Effects on Experimental Acute Aortic Insufficiency." *Annals of Thoracic Surg.*, 21(2): 134-136, Feb. 1976.

Sochman et al., "Percutaneous Transcatheter Aortic Disc Valve Prosthesis Implantation: A Feasibility Study." *Cardiovasc. Intervent. Radiol.*, 23: 384-388, Sep. 2000.

Stuart, "In Heart Valves, A Brave, New Non-Surgical World." *Start-Up*. Feb. 9-17, 2004.

Stassano. "Mid-term Results of the Valve-on-Valve Technique for Bioprosthetic Failure." *European Journal of Cardiothoracic Surgery*: vol. 18, 453-457, Oct. 2000.

"A Matter of Size." Triennial Review of the National Nanotechnology Initiative, The National Academies Press, Washington DC, v-13, <http://www.nap.edu/catalog/11752/a-matter-of-size-triennial-review-of-the-national-nanotechnology>, 2006.

Cunanan et al., "Tissue Characterization and Calcification Potential of Commercial Bioprosthetic Heart Valves." *Ann. Thorac. Surg.*, S417-421, May 15, 2001.

"Heart Valve Materials—Bovine (cow)." Equine & Porcine Pericardium, Maverick Biosciences Pty. Lt, <http://maverickbio.com/biological-medical-device-materials.php?htm>. 2009.

Laborde et al., "Percutaneous Implantation of the Corevalve Aortic Valve Prosthesis for Patients Presenting High Risk for Surgical Valve Replacement." *EuroIntervention*: 472-474, Feb. 2006.

Vahanian et al., "Percutaneous Approaches to Valvular Disease." *Circulation*, 109: 1572-1579, Apr. 6, 2004.

Van Herwerden et al., "Percutaneous Valve Implantation: Back to the Future?" *Euro. Heart J.*, 23(18): 1415-1416, Sep. 2002.

Zhou et al., "Self-expandable Valved Stent of Large Size: Off-Bypass Implantation in Pulmonary Position." *Eur. J. Cardiothorac.*, 24: 212-216, Aug. 2003.

International Search Report and Written Opinion dated Feb. 13, 2017 for International Application No. PCT/US2016/015288.

* cited by examiner

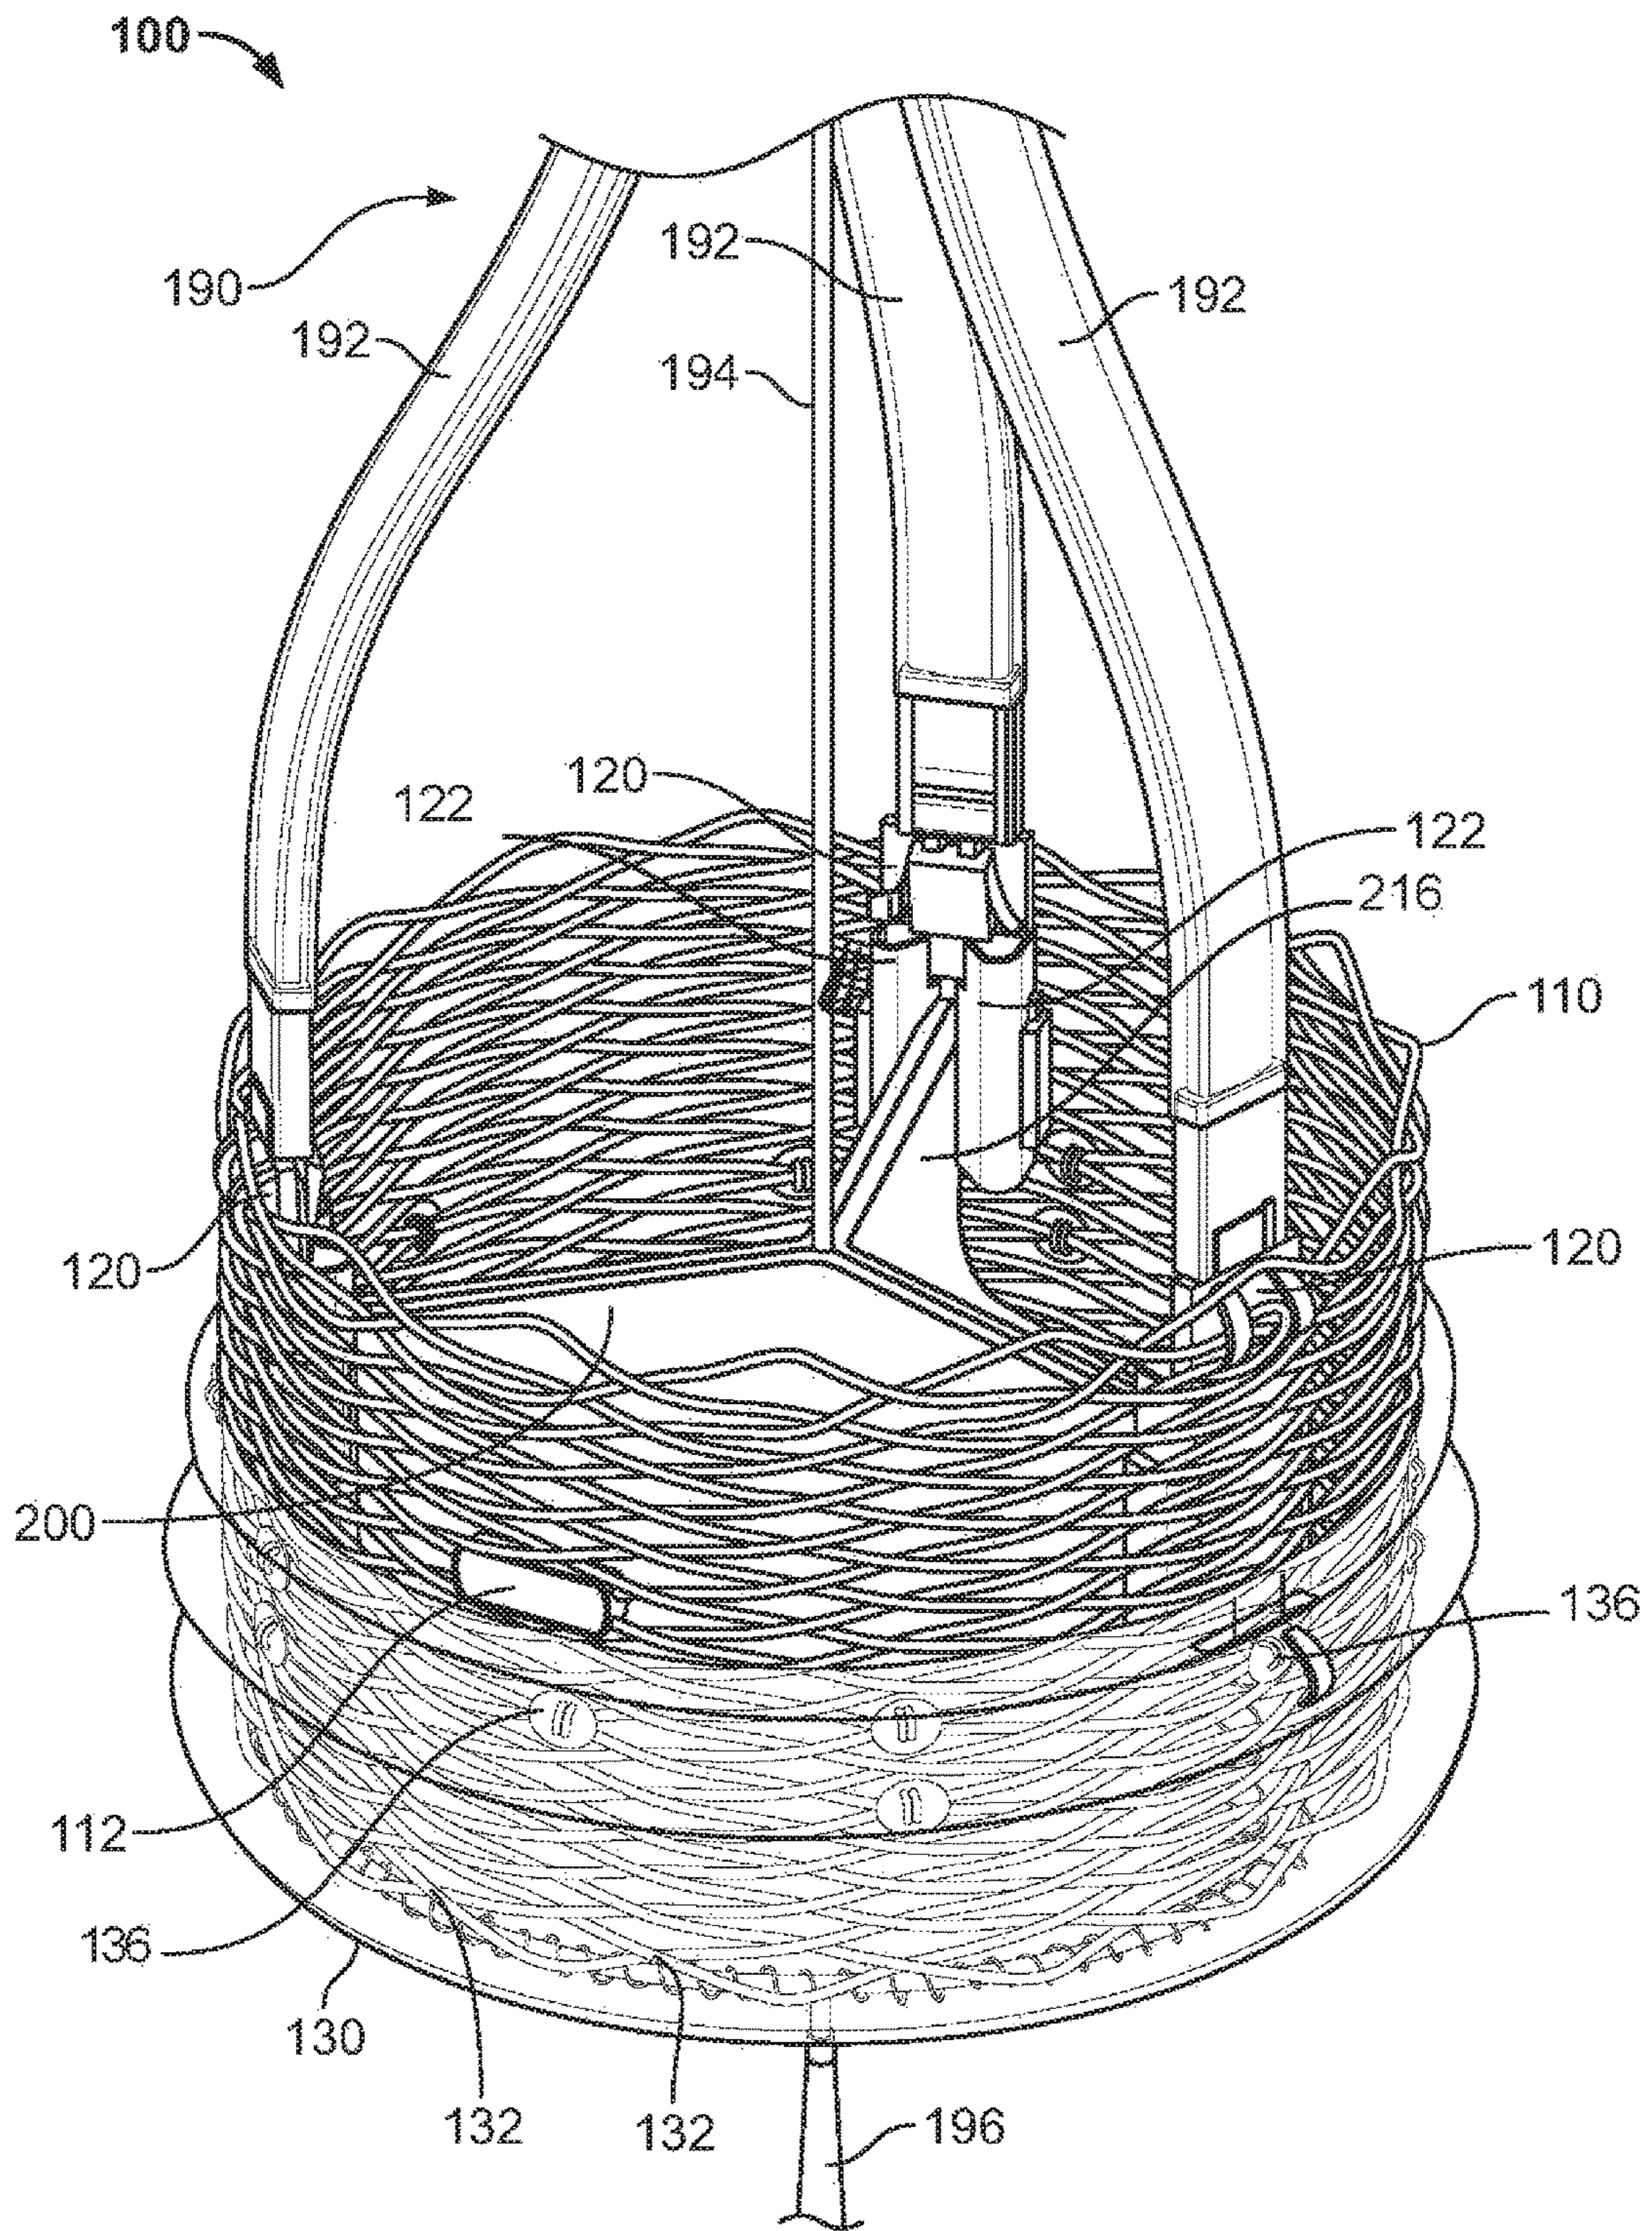


FIG. 1A

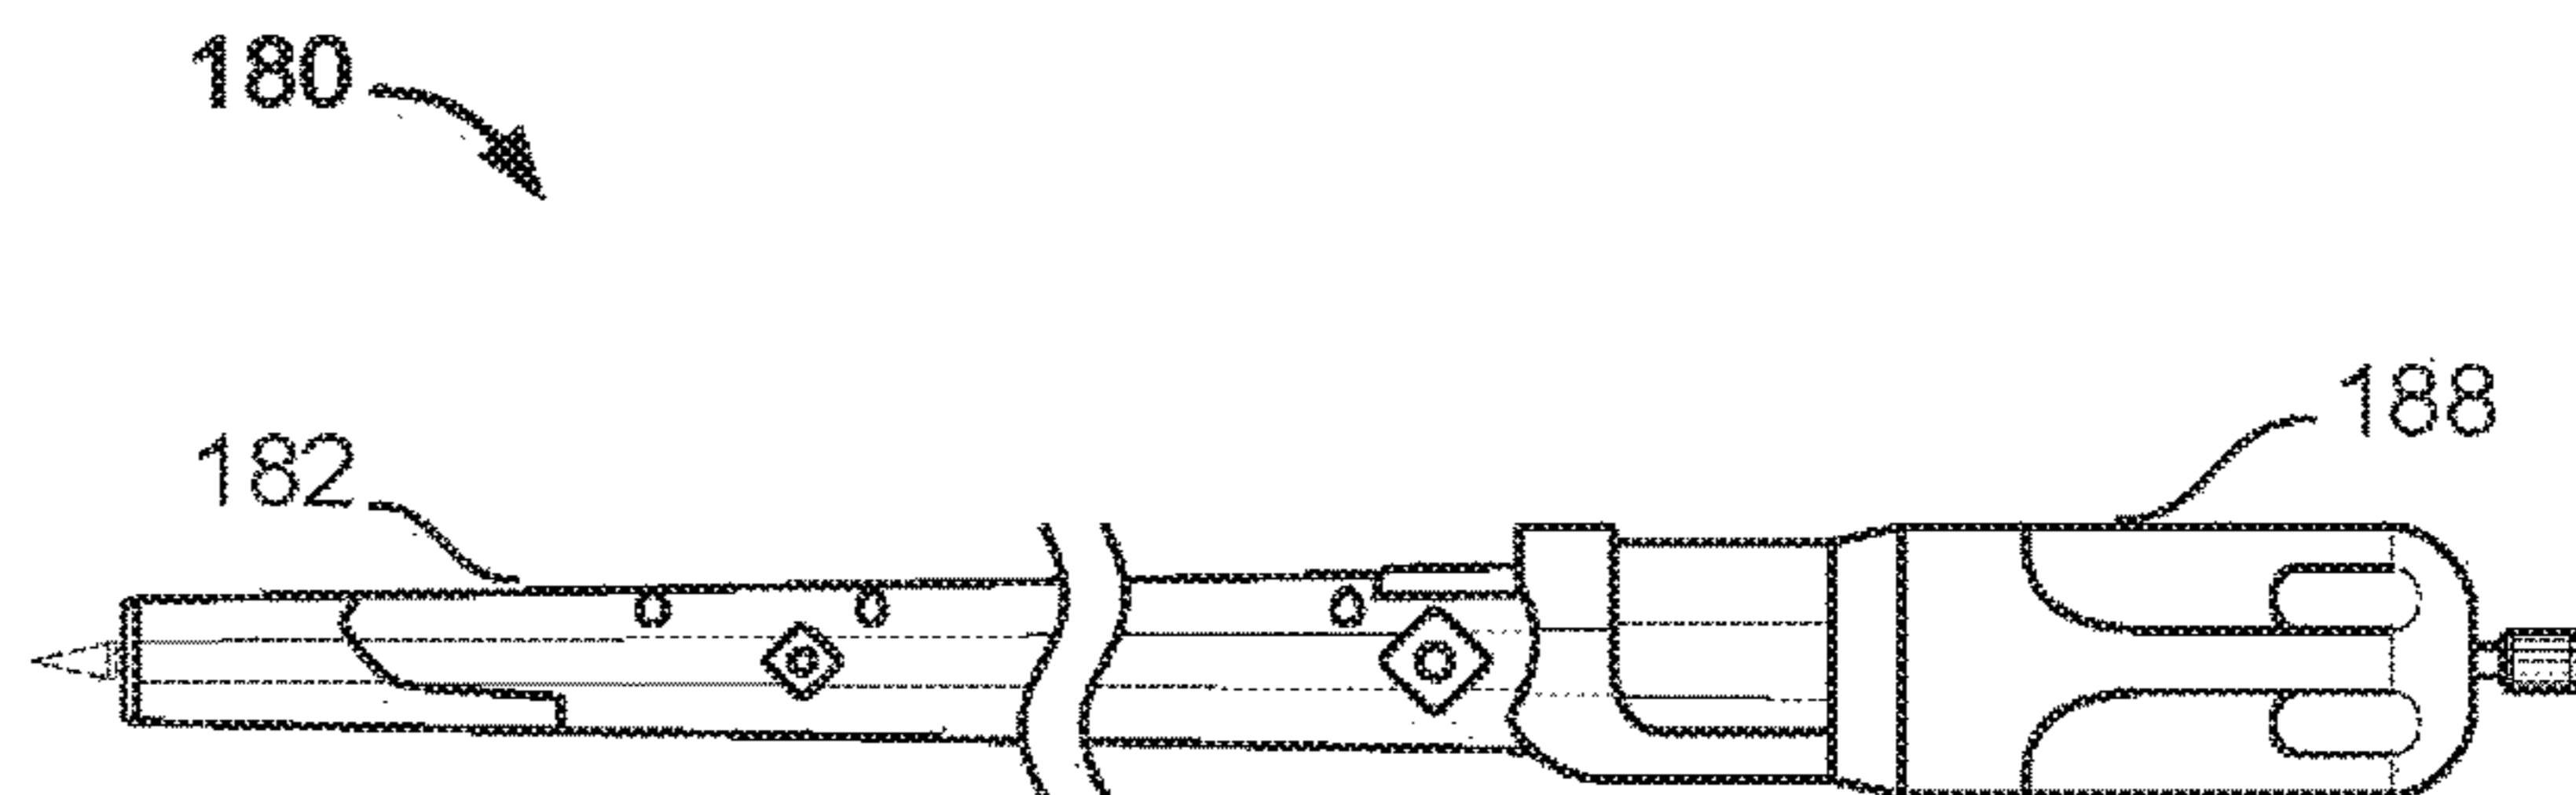


FIG. 1C

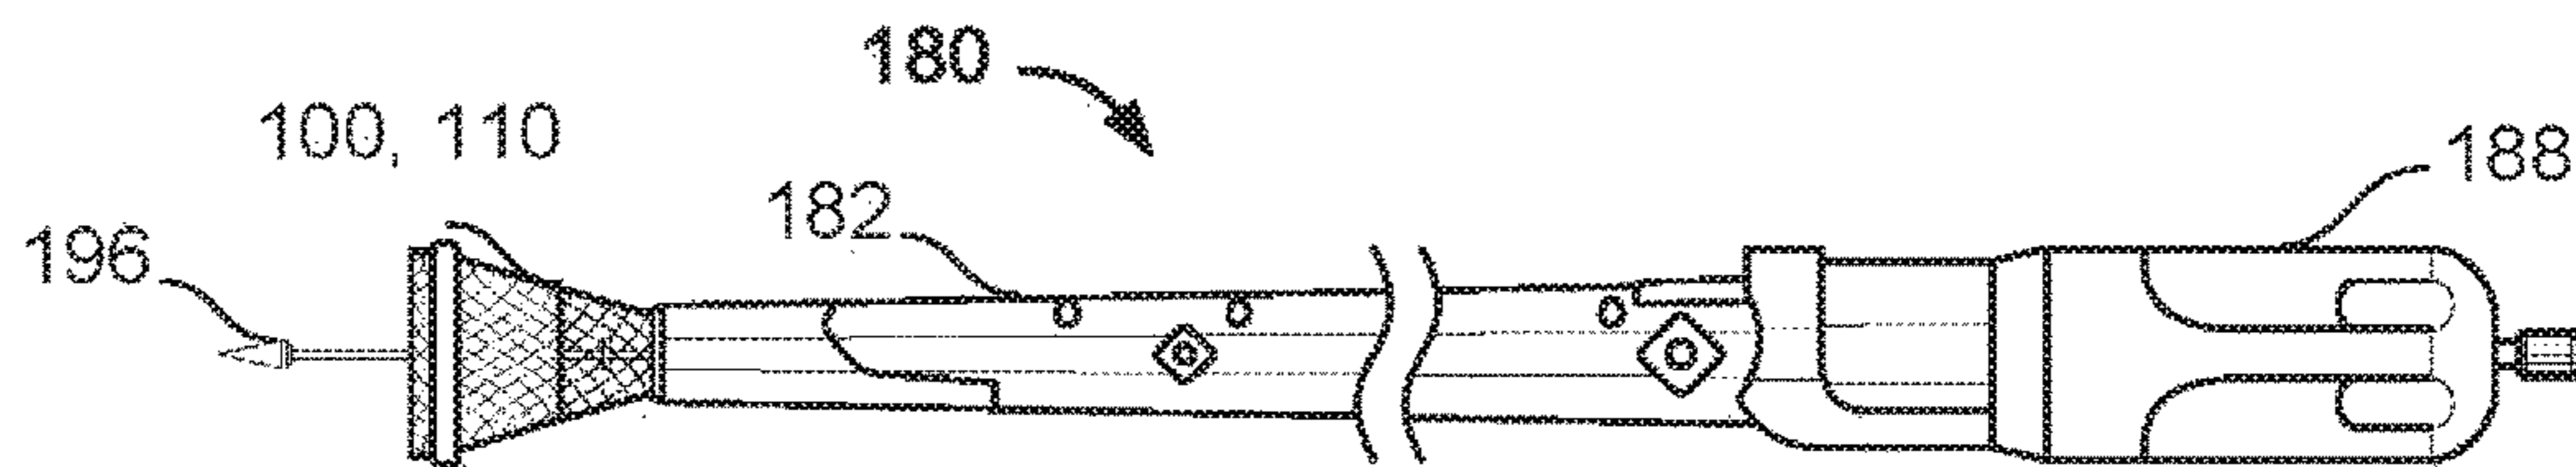


FIG. 1D

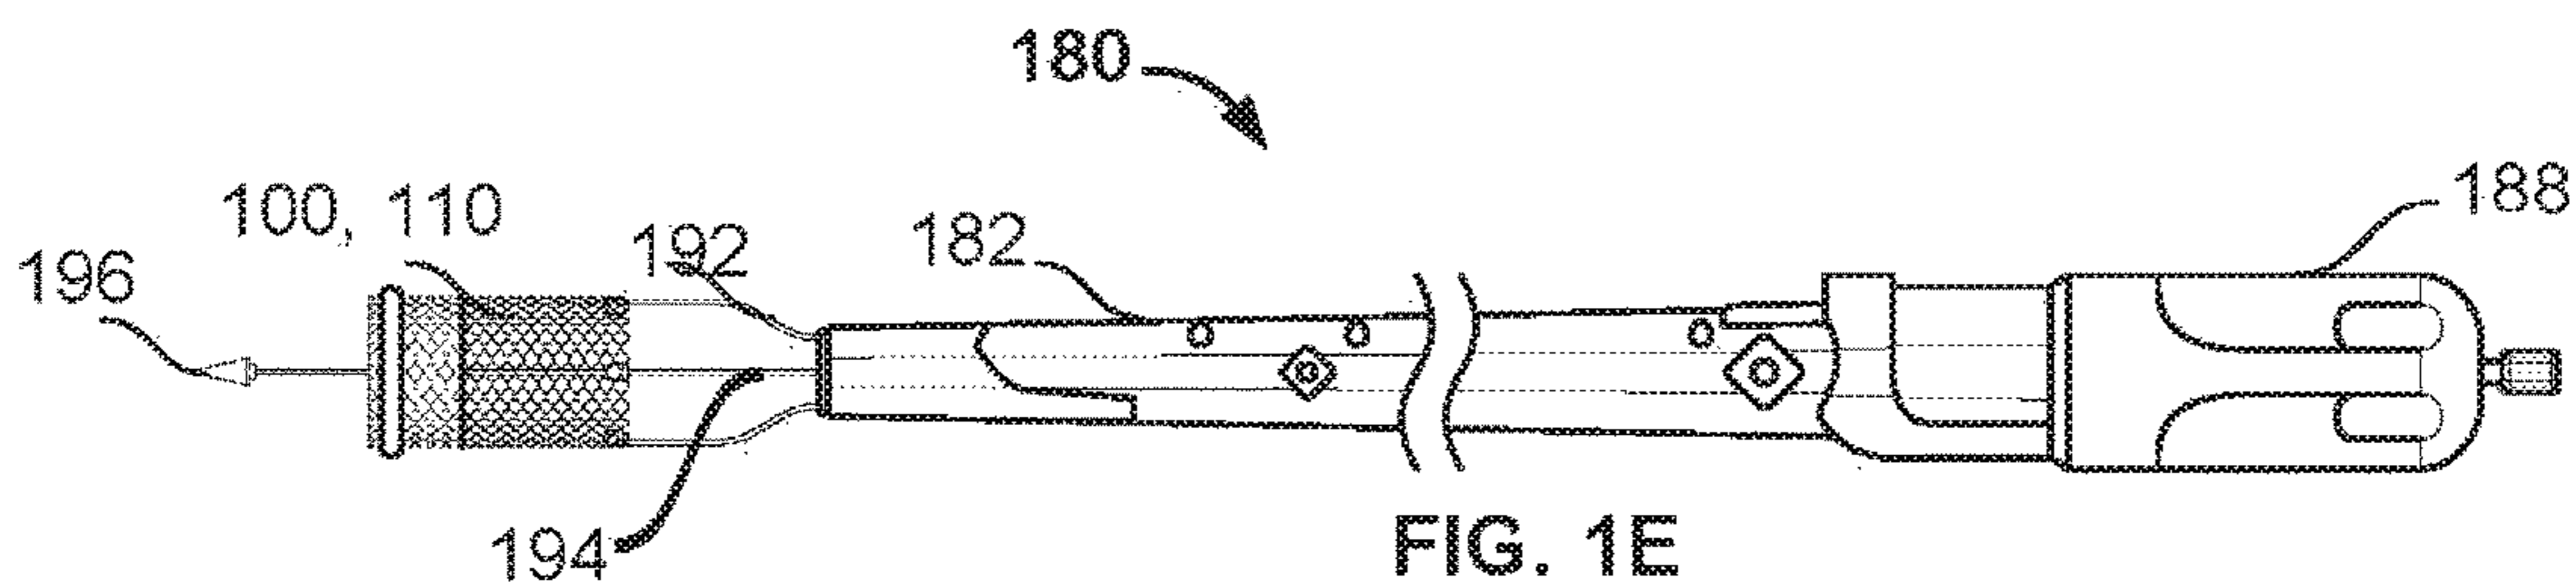


FIG. 1E

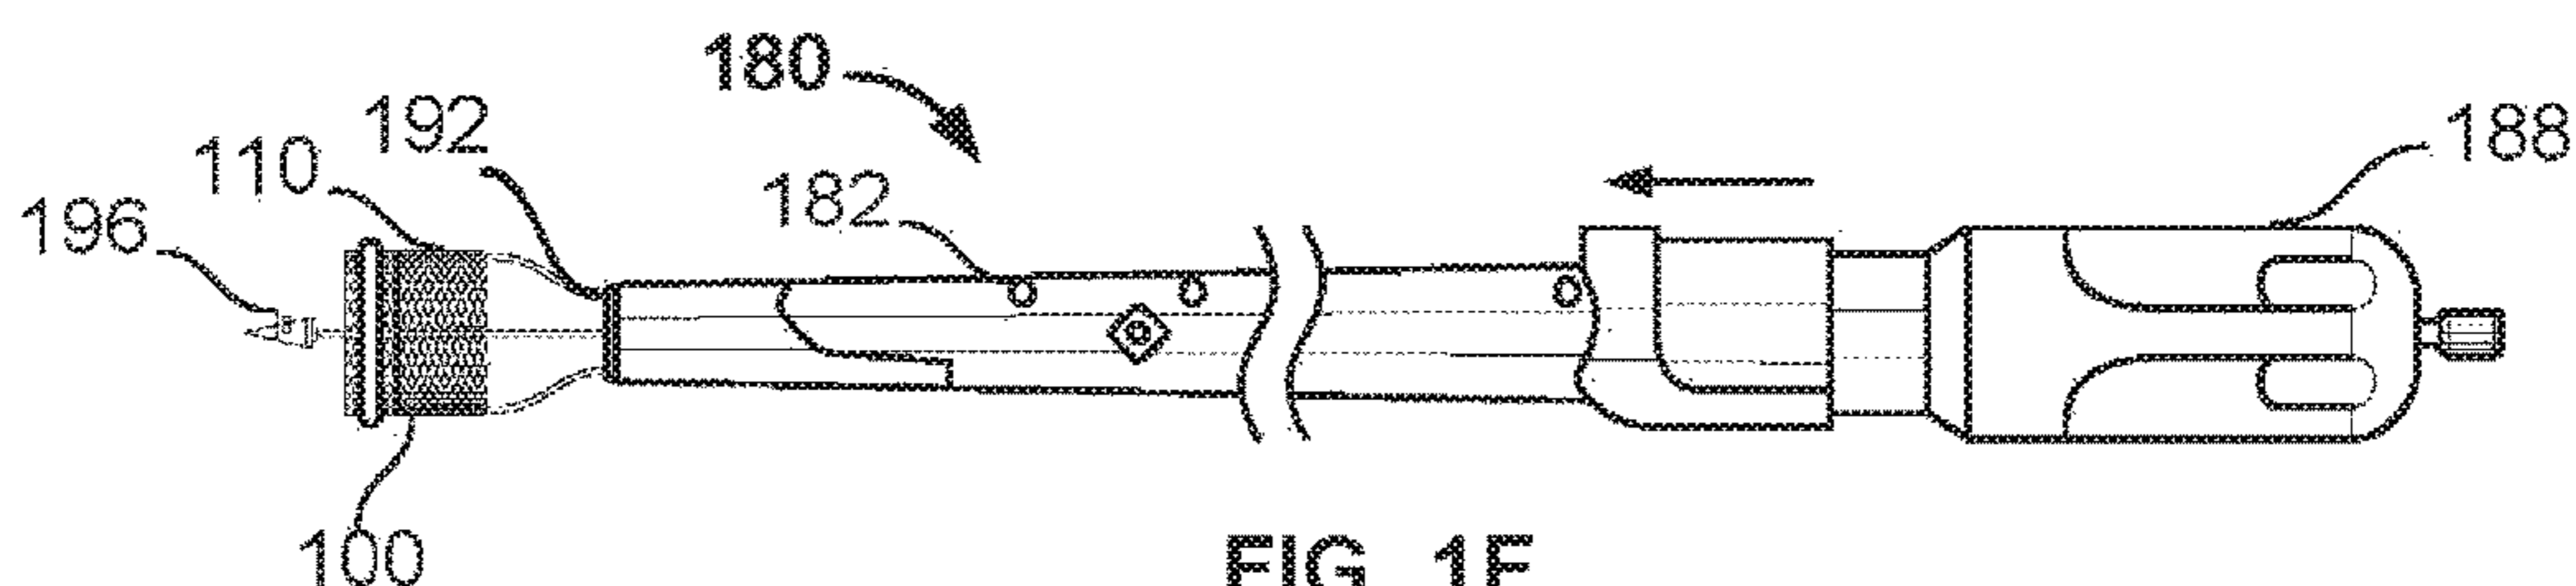


FIG. 1F

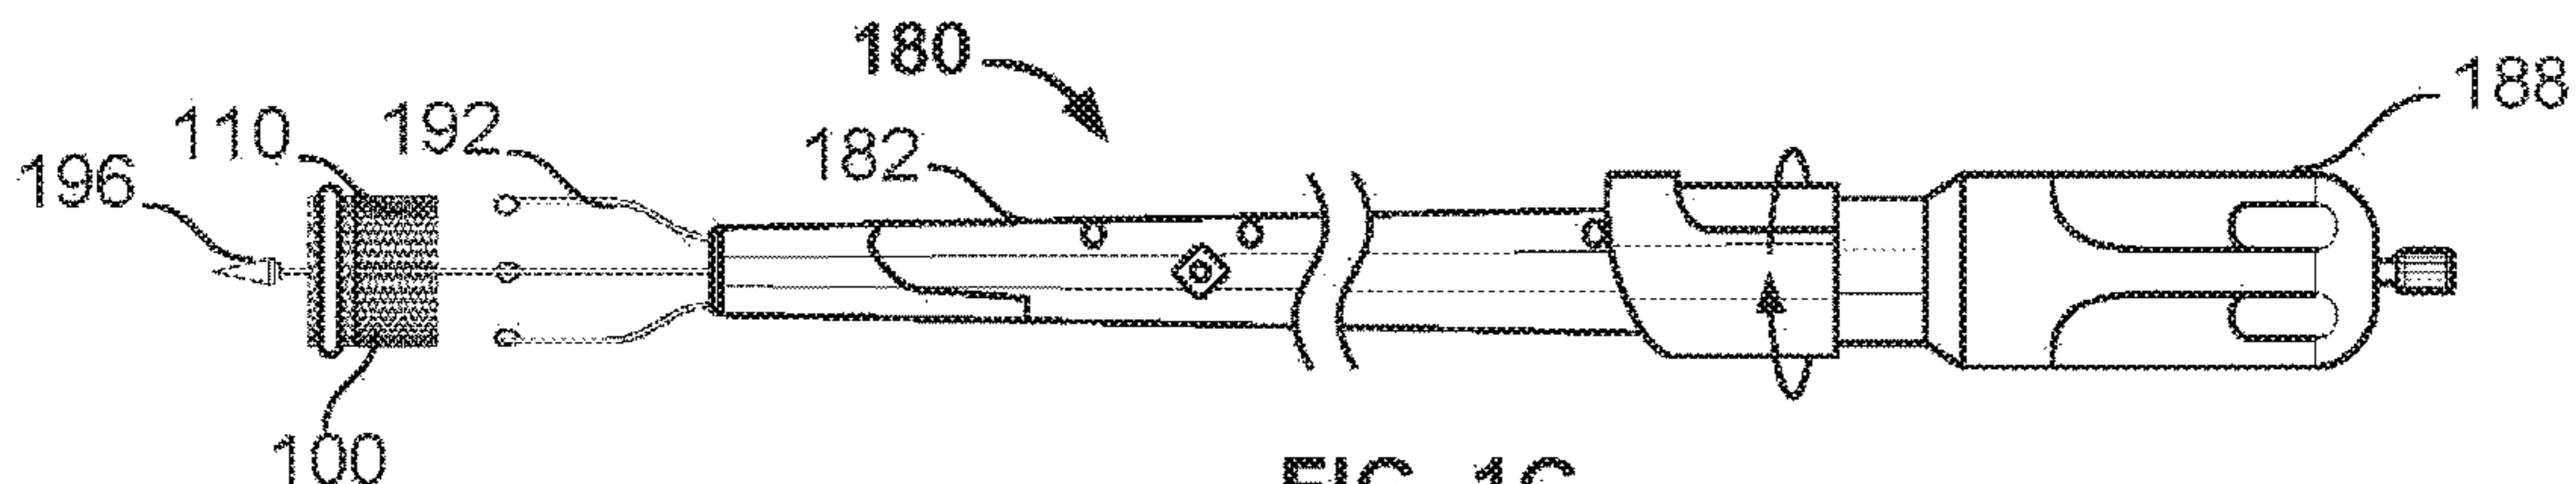


FIG. 1G

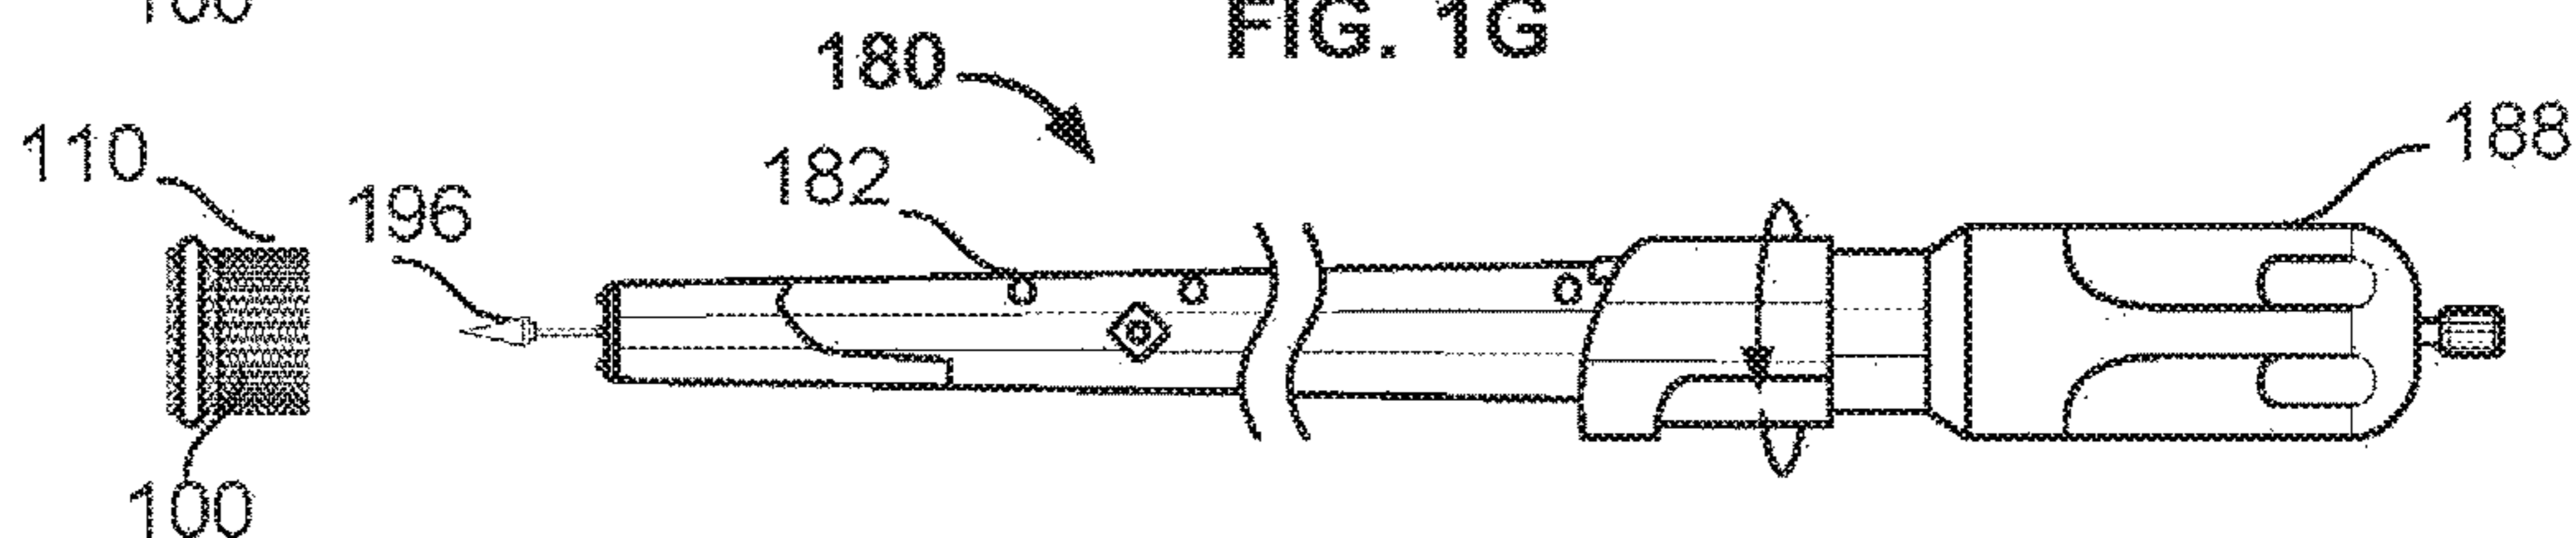


FIG. 1H

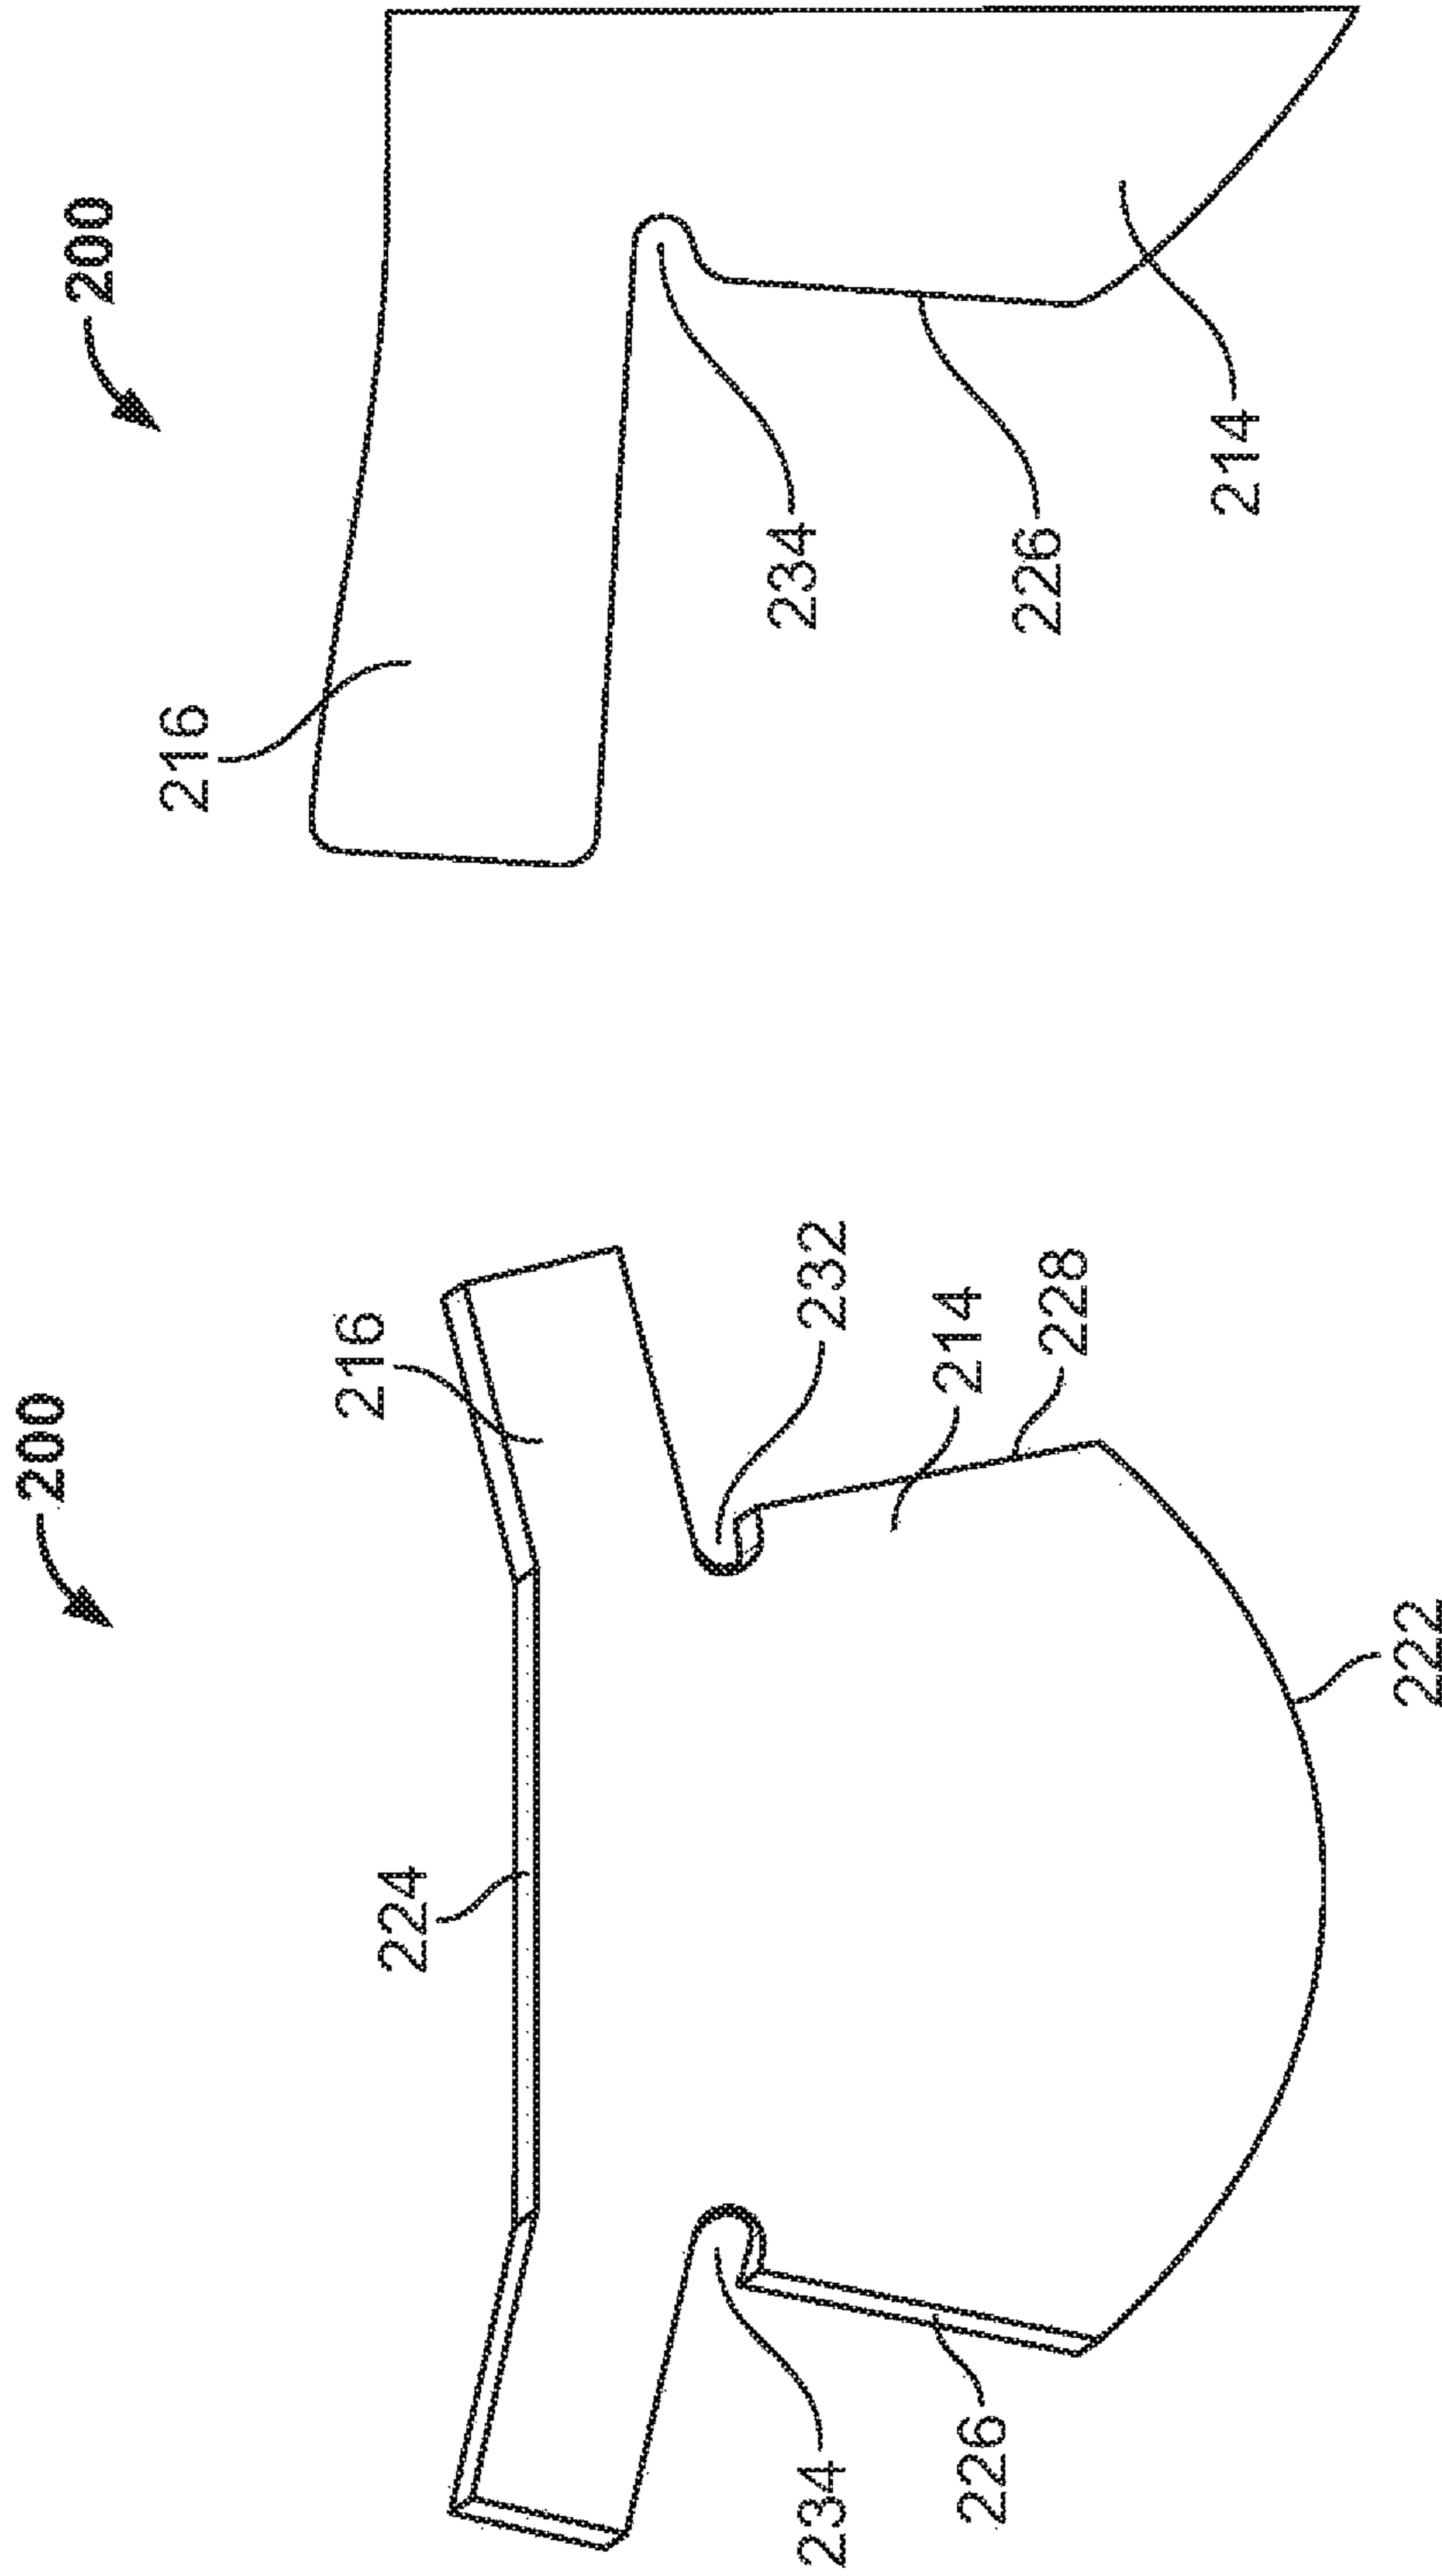


FIG. 2B

FIG. 2A

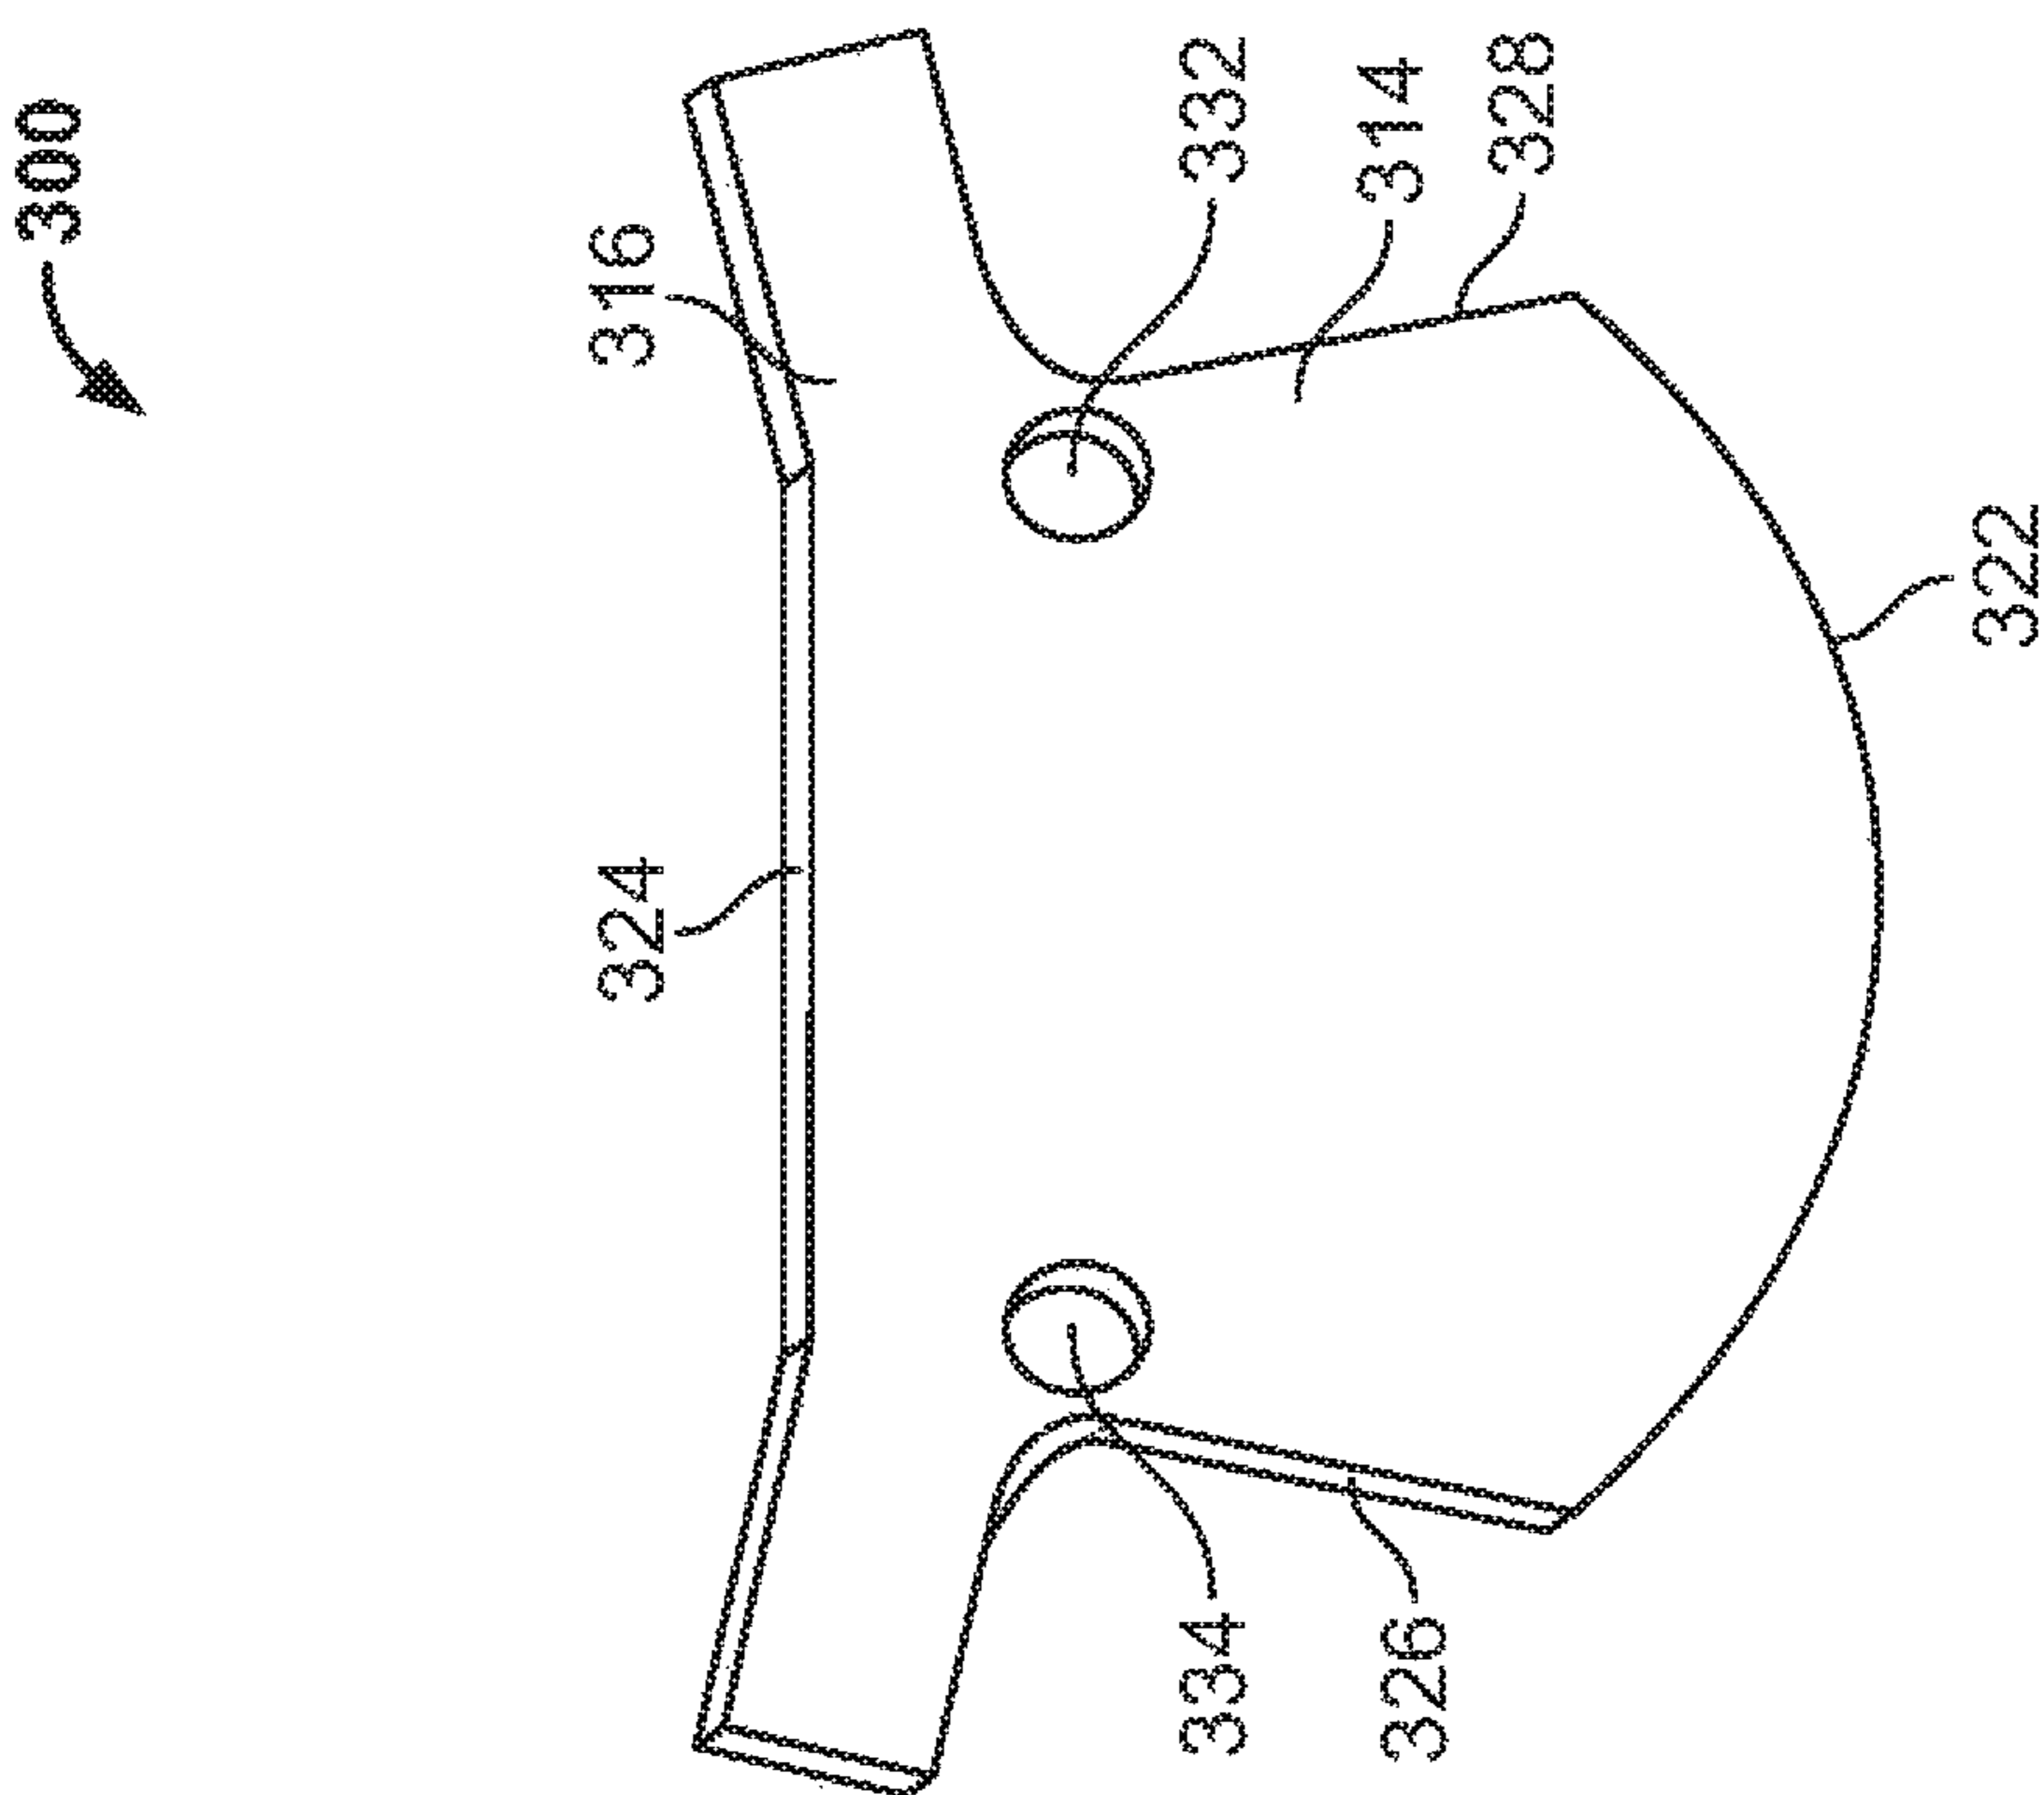


FIG. 3

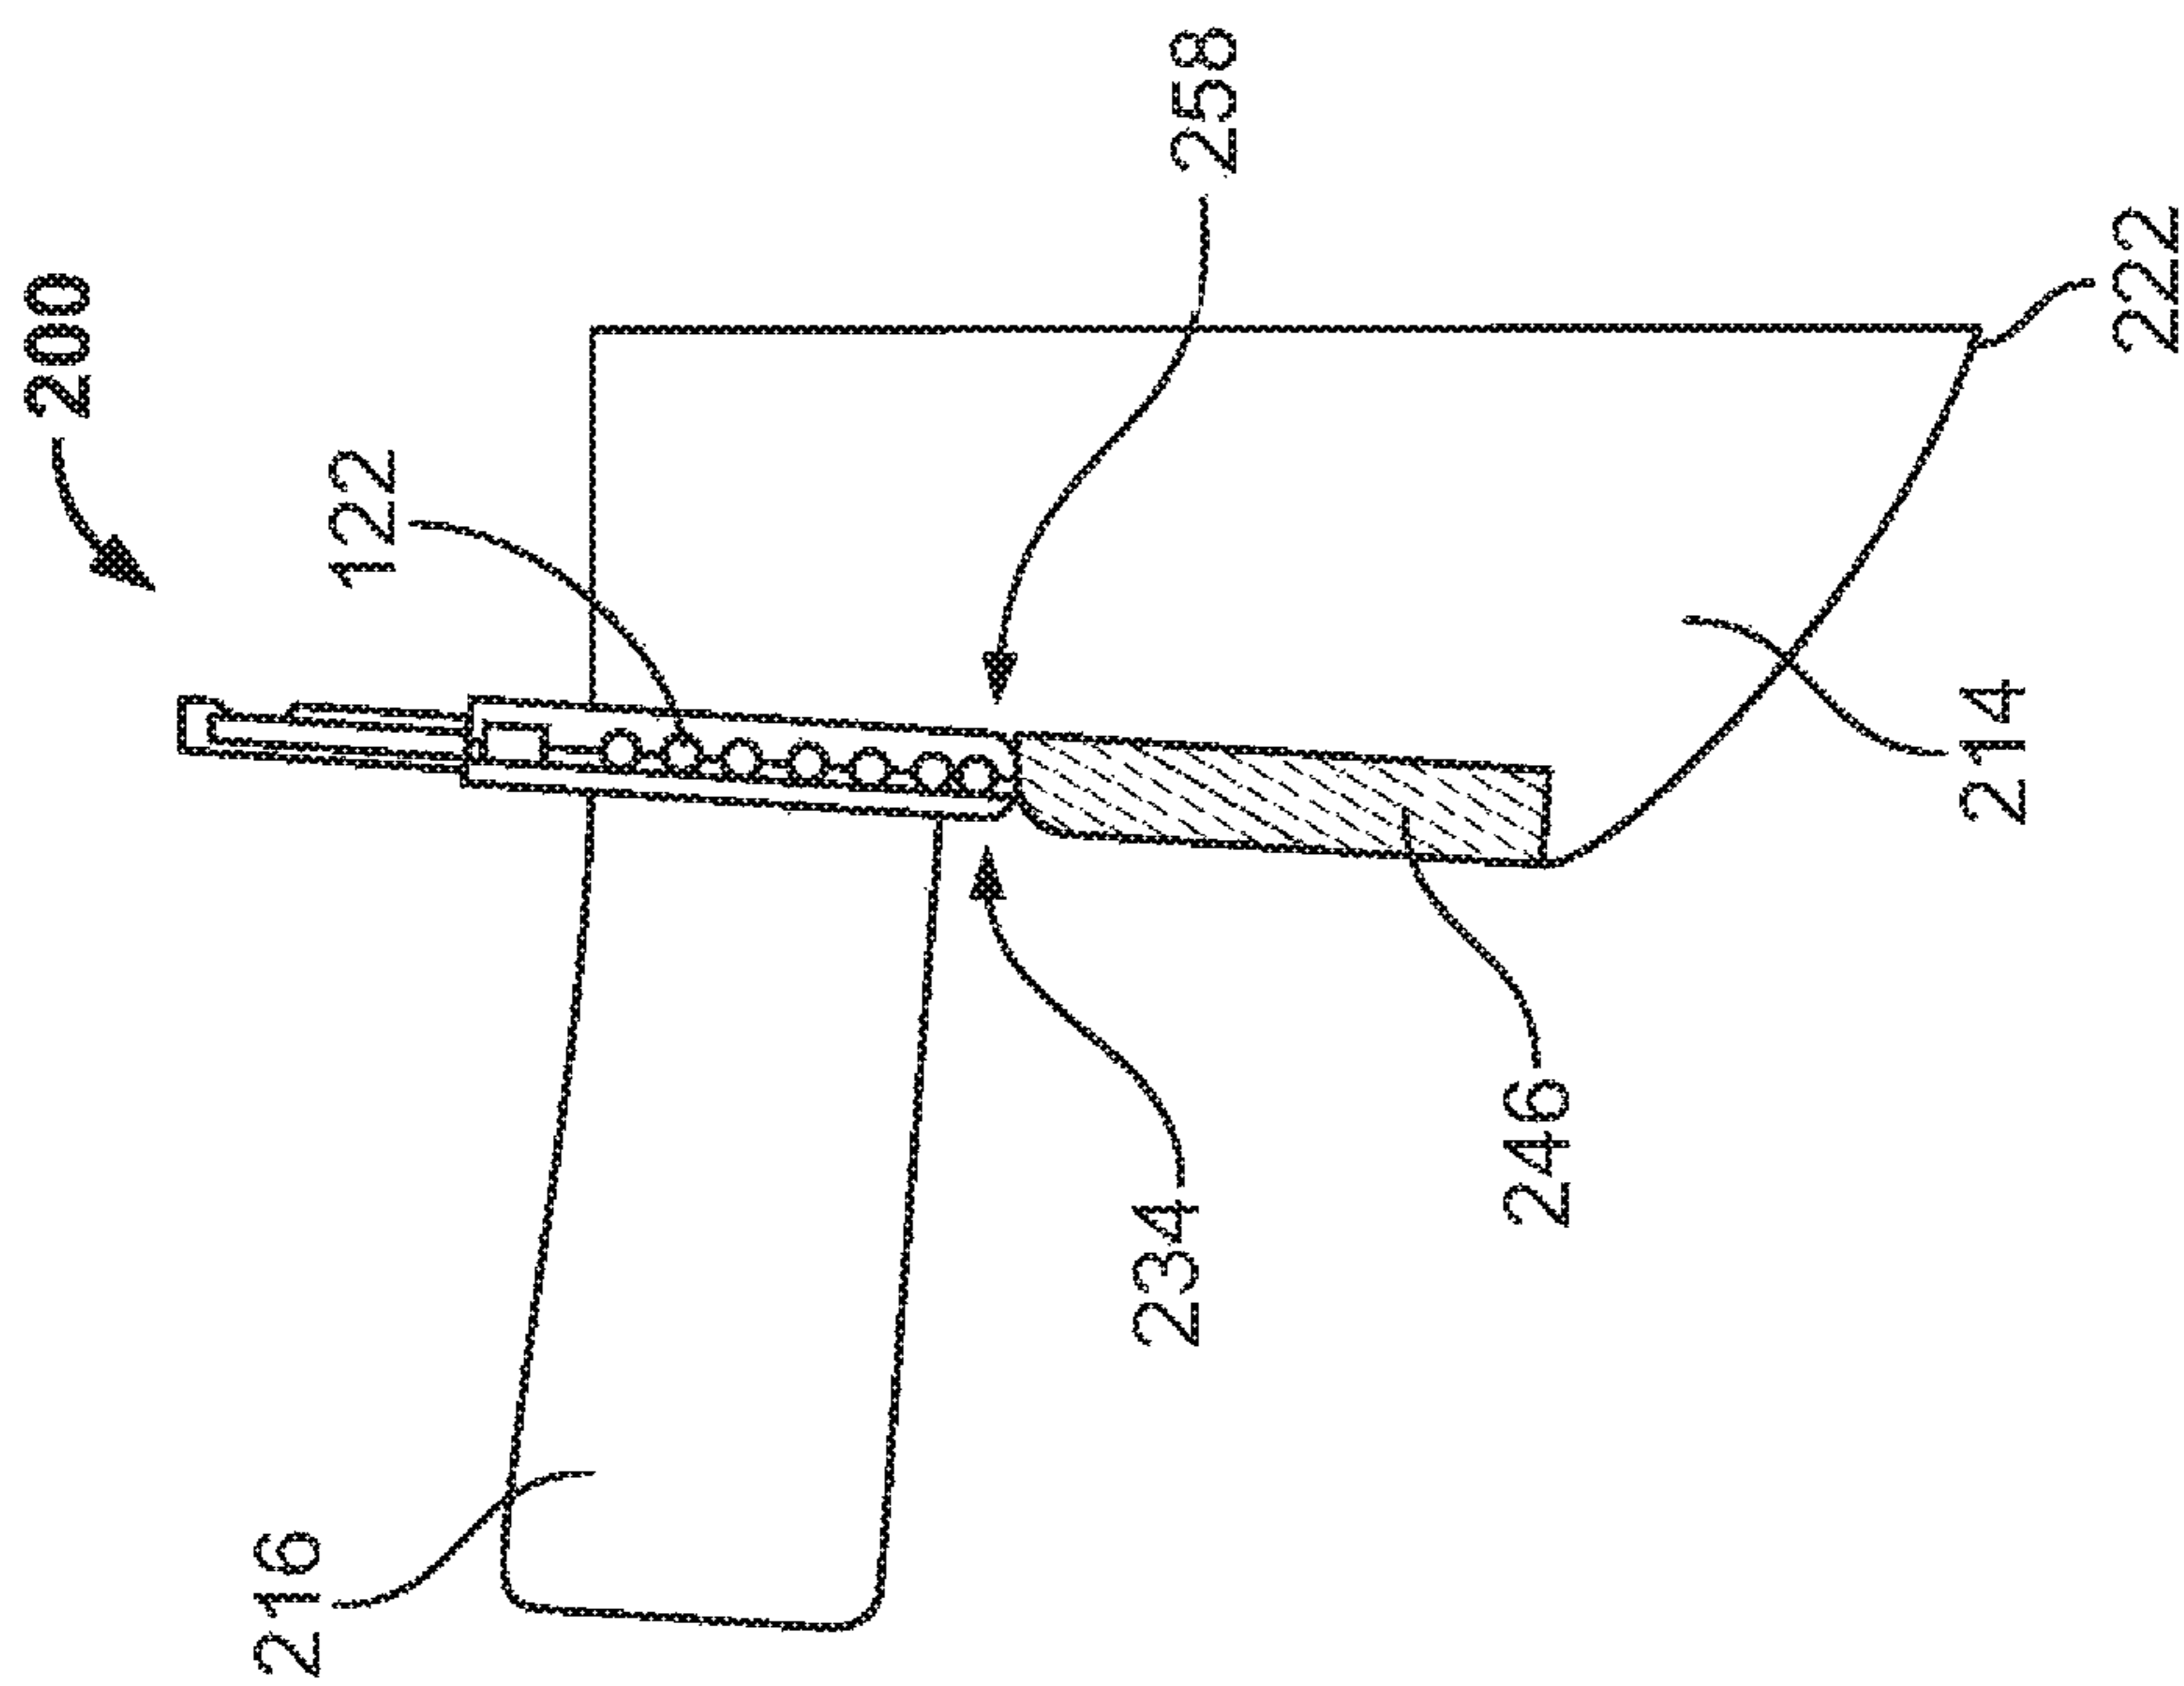


FIG. 2C

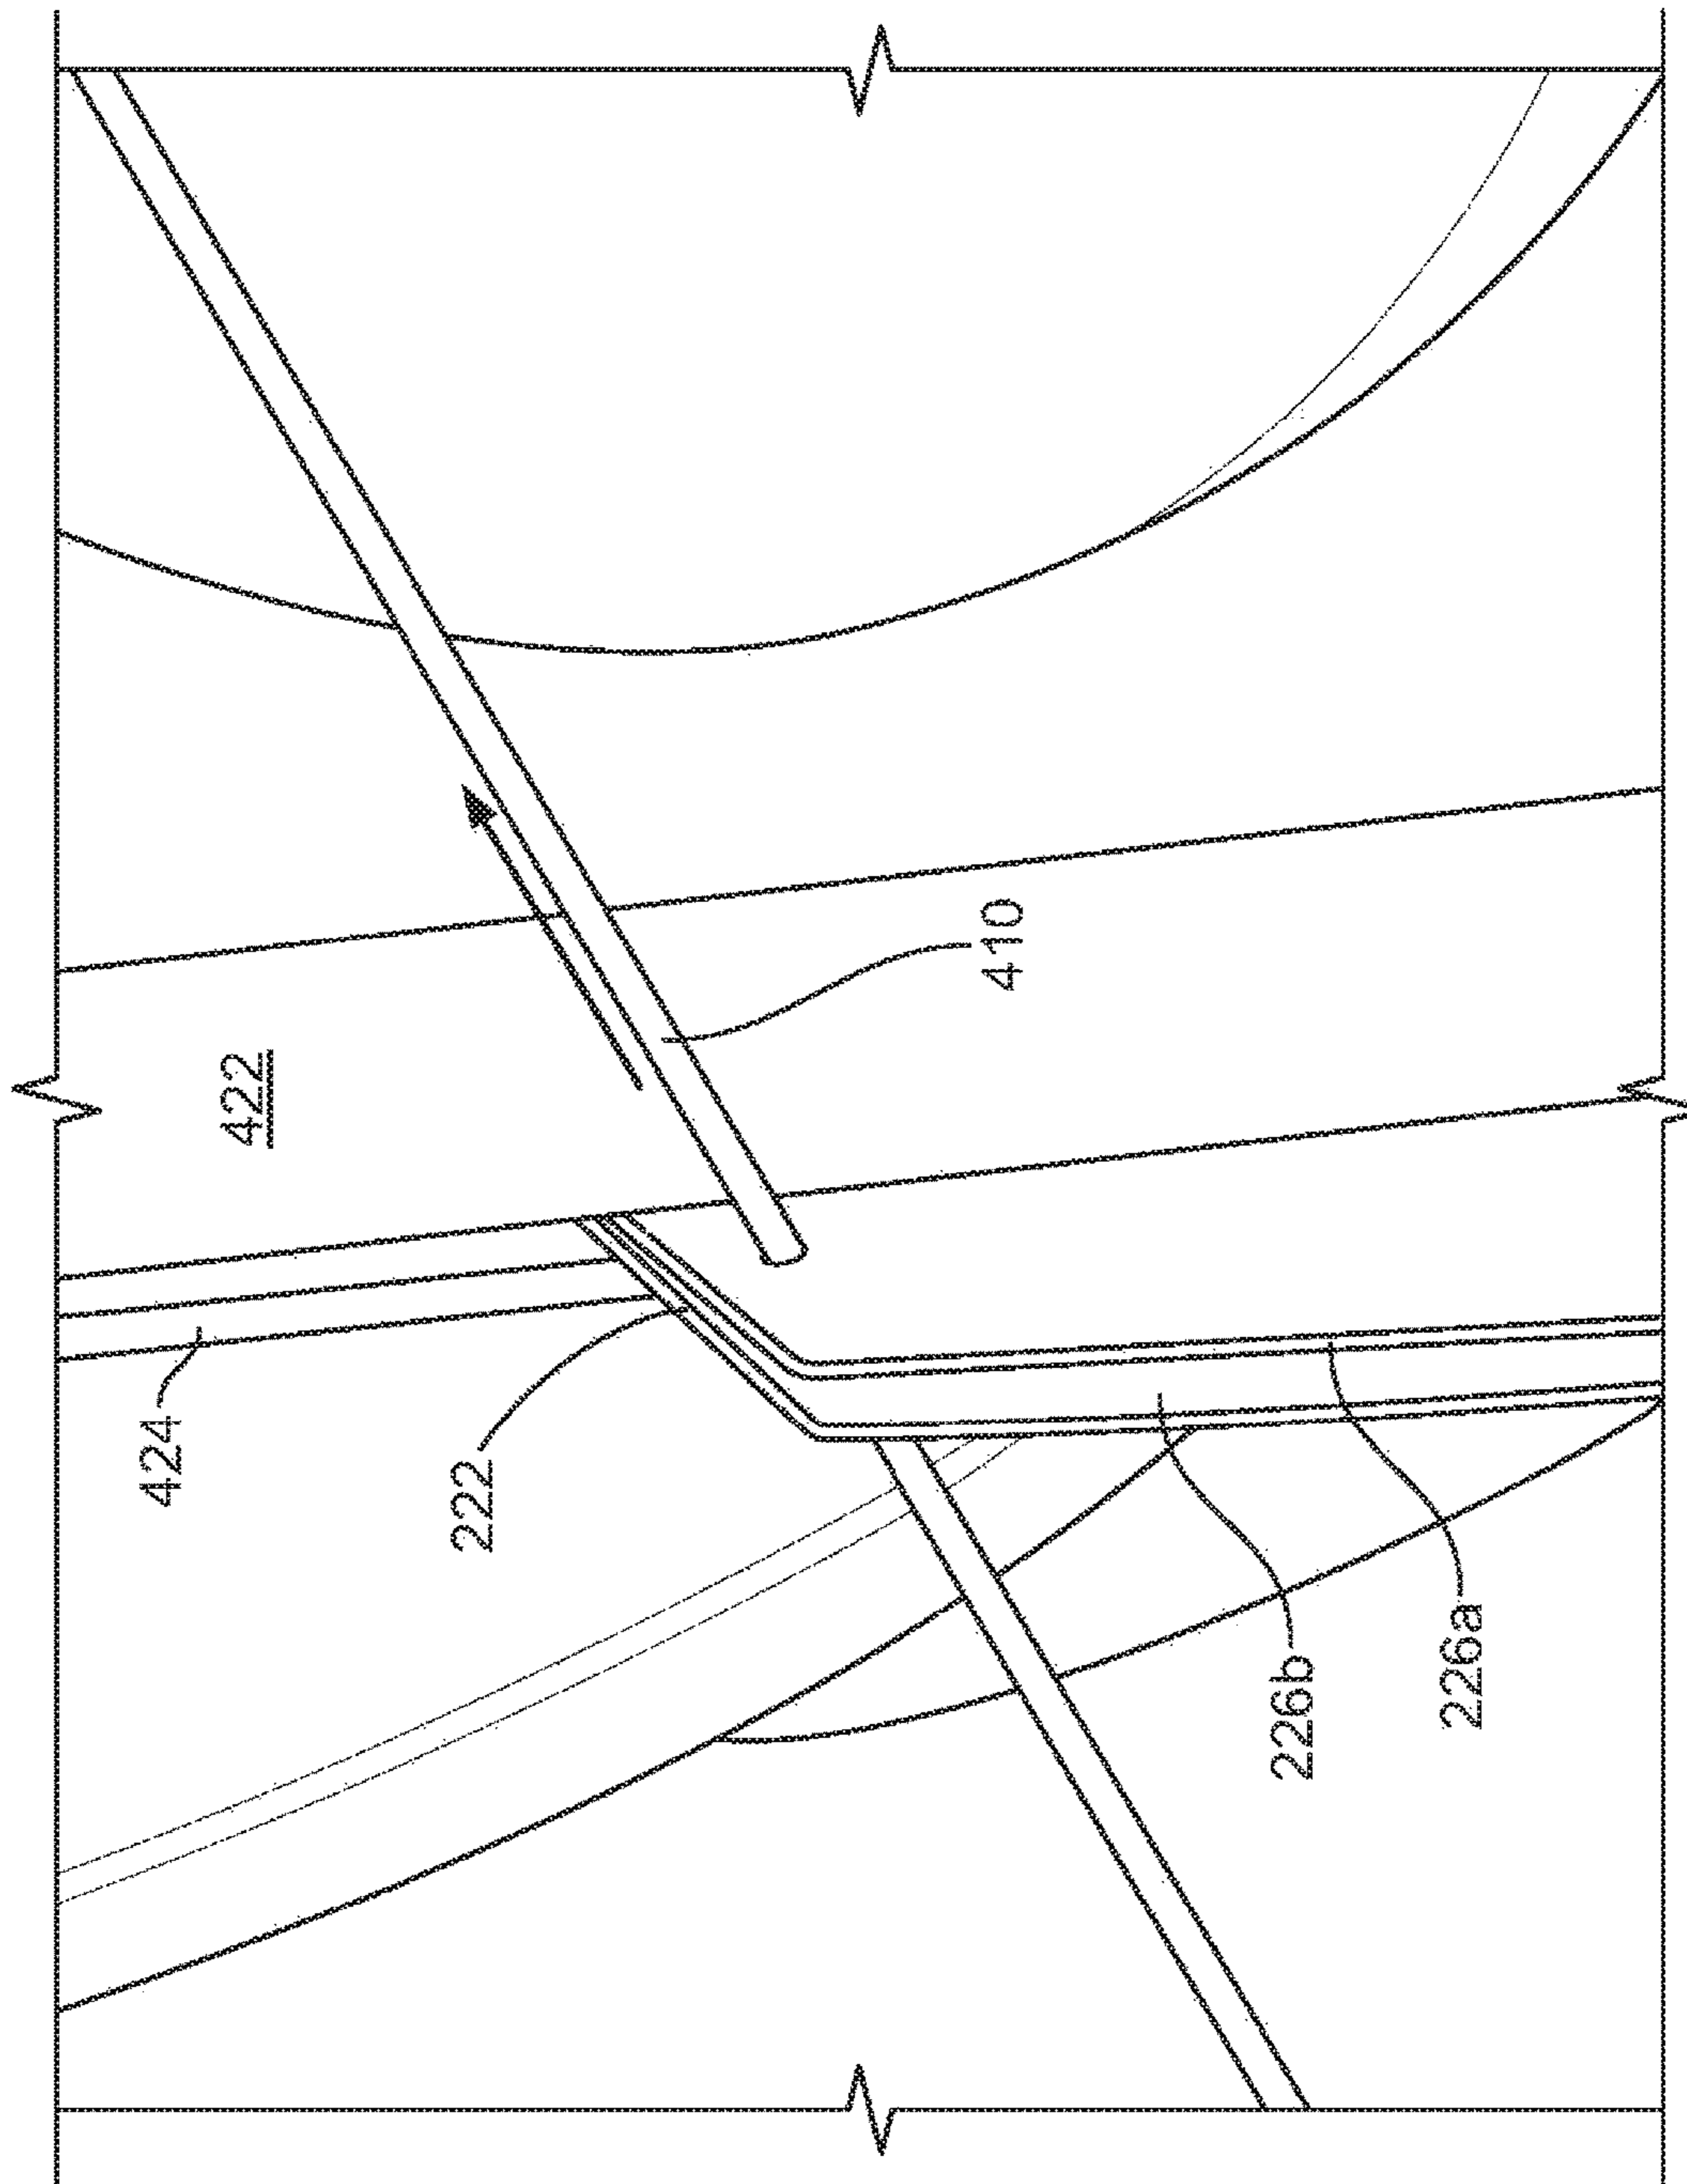


FIG. 4A

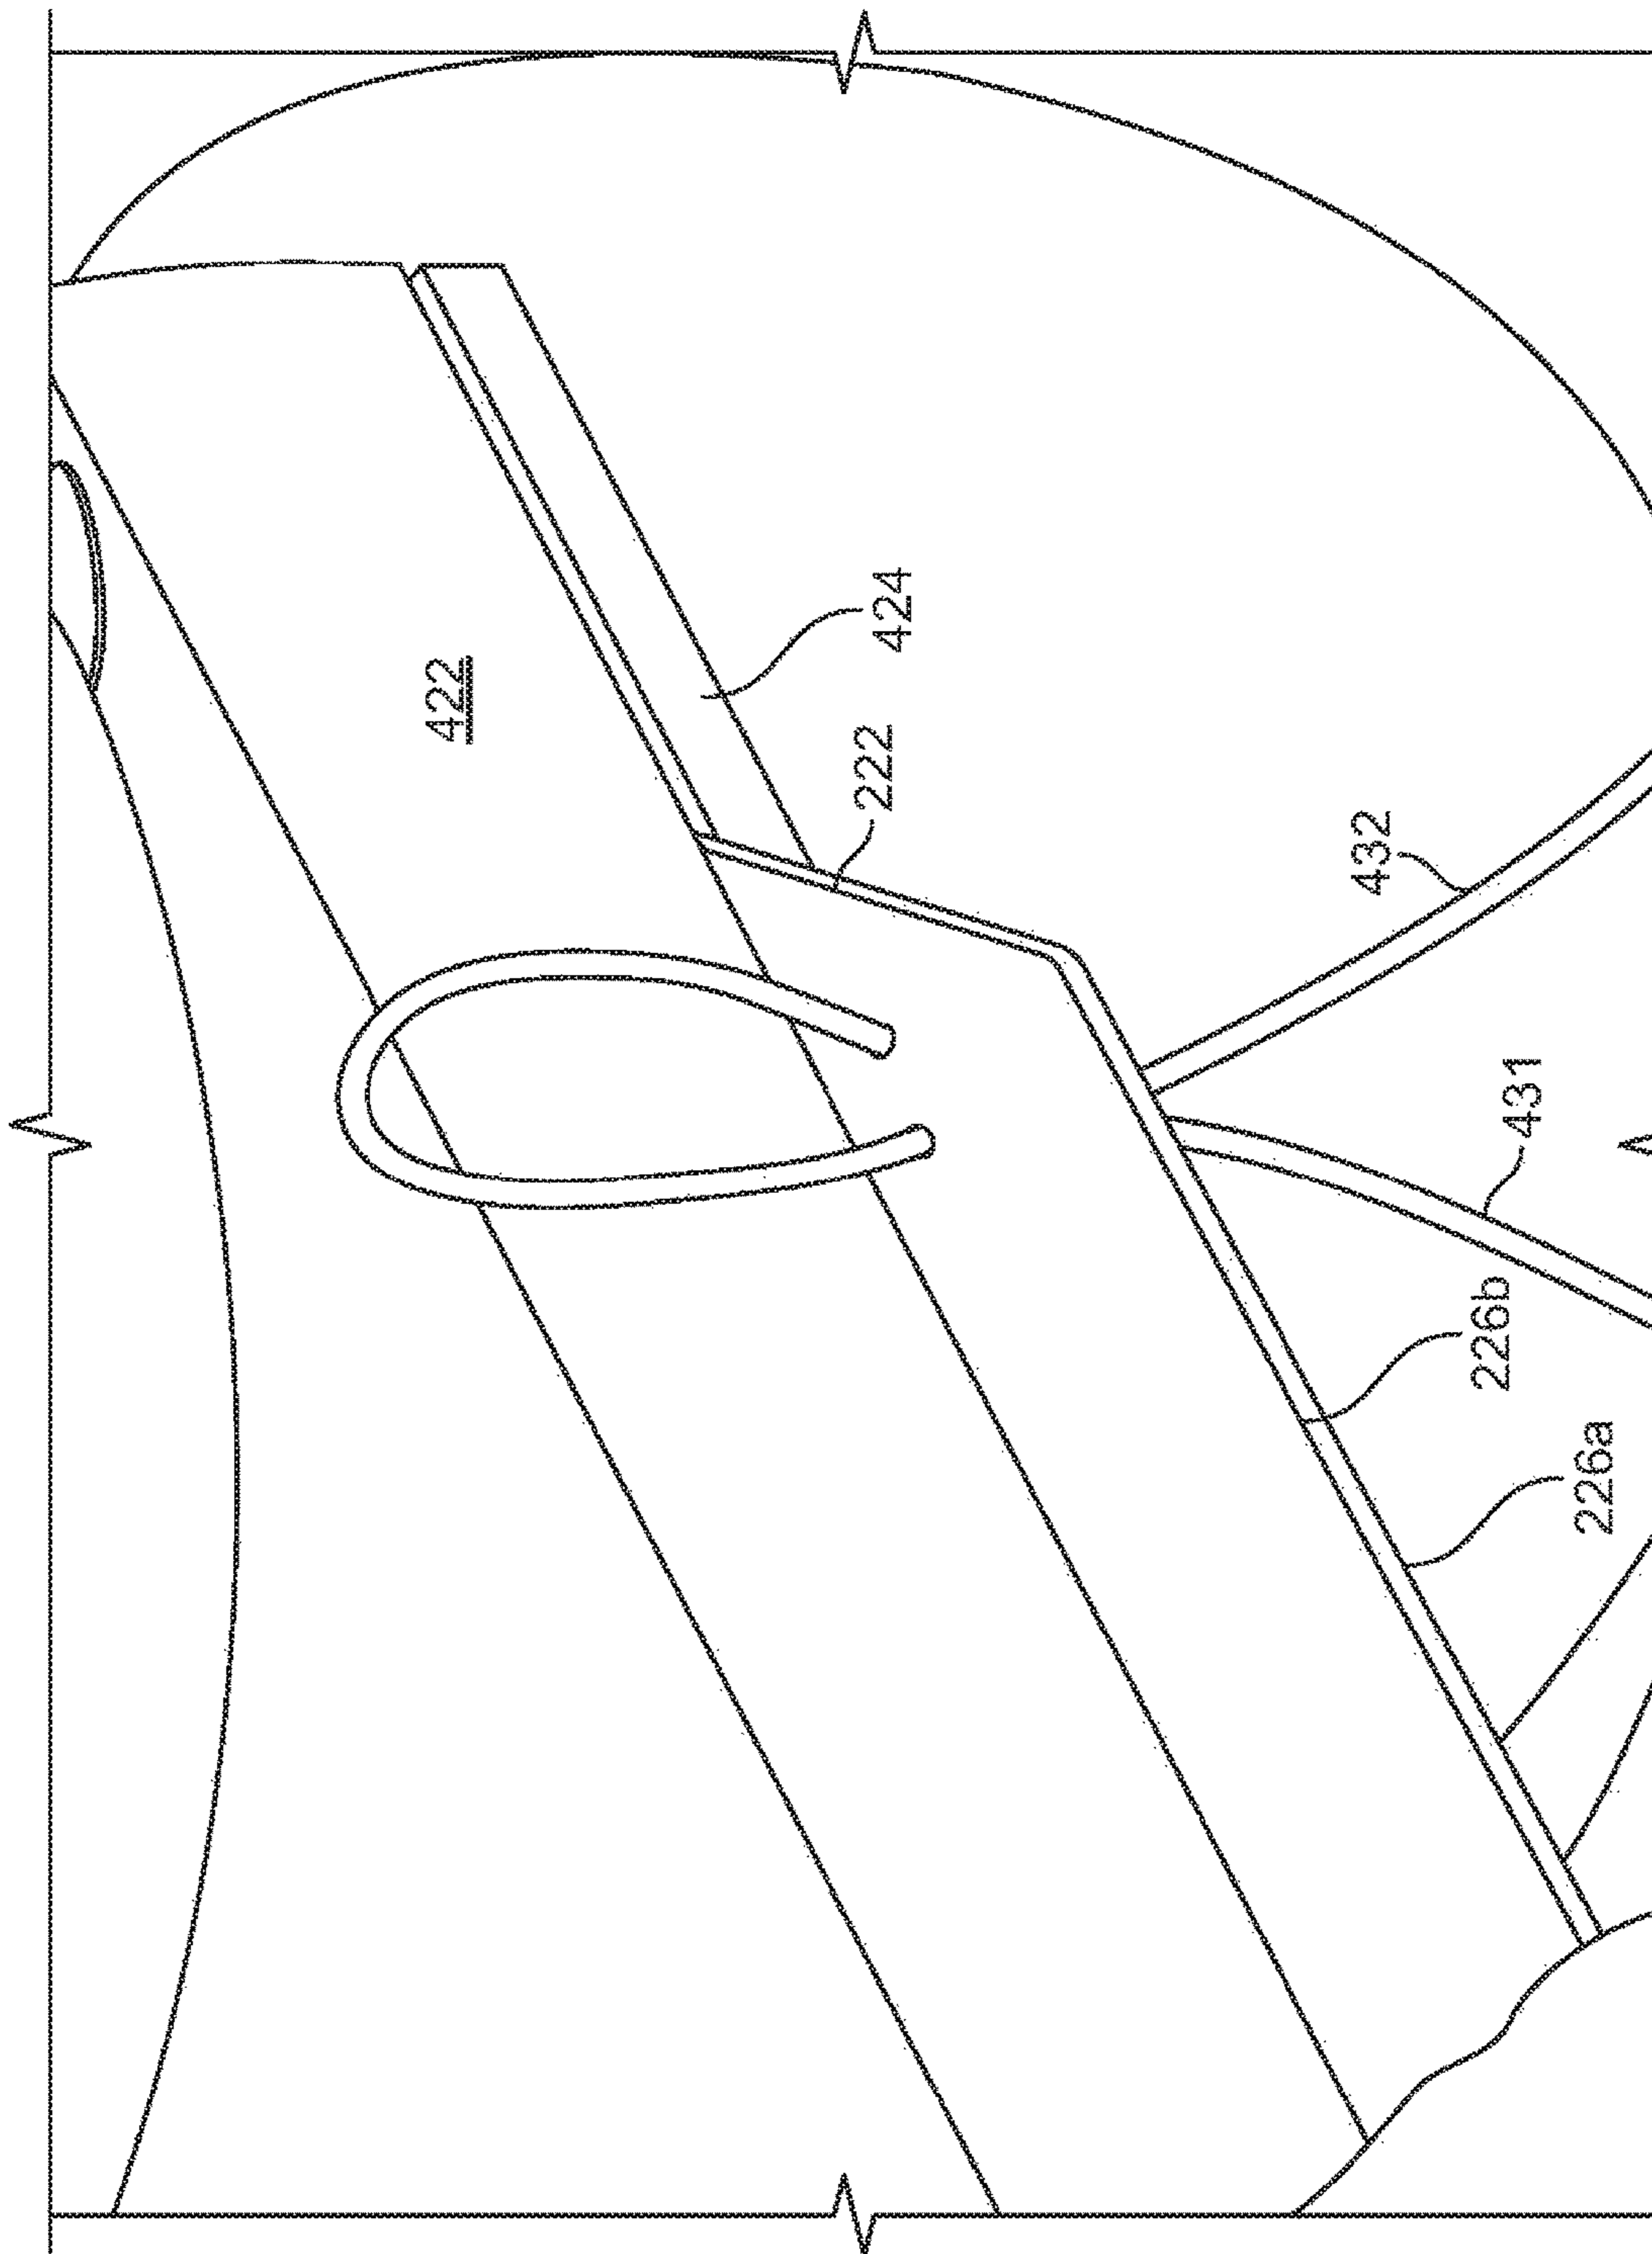


FIG. 4B

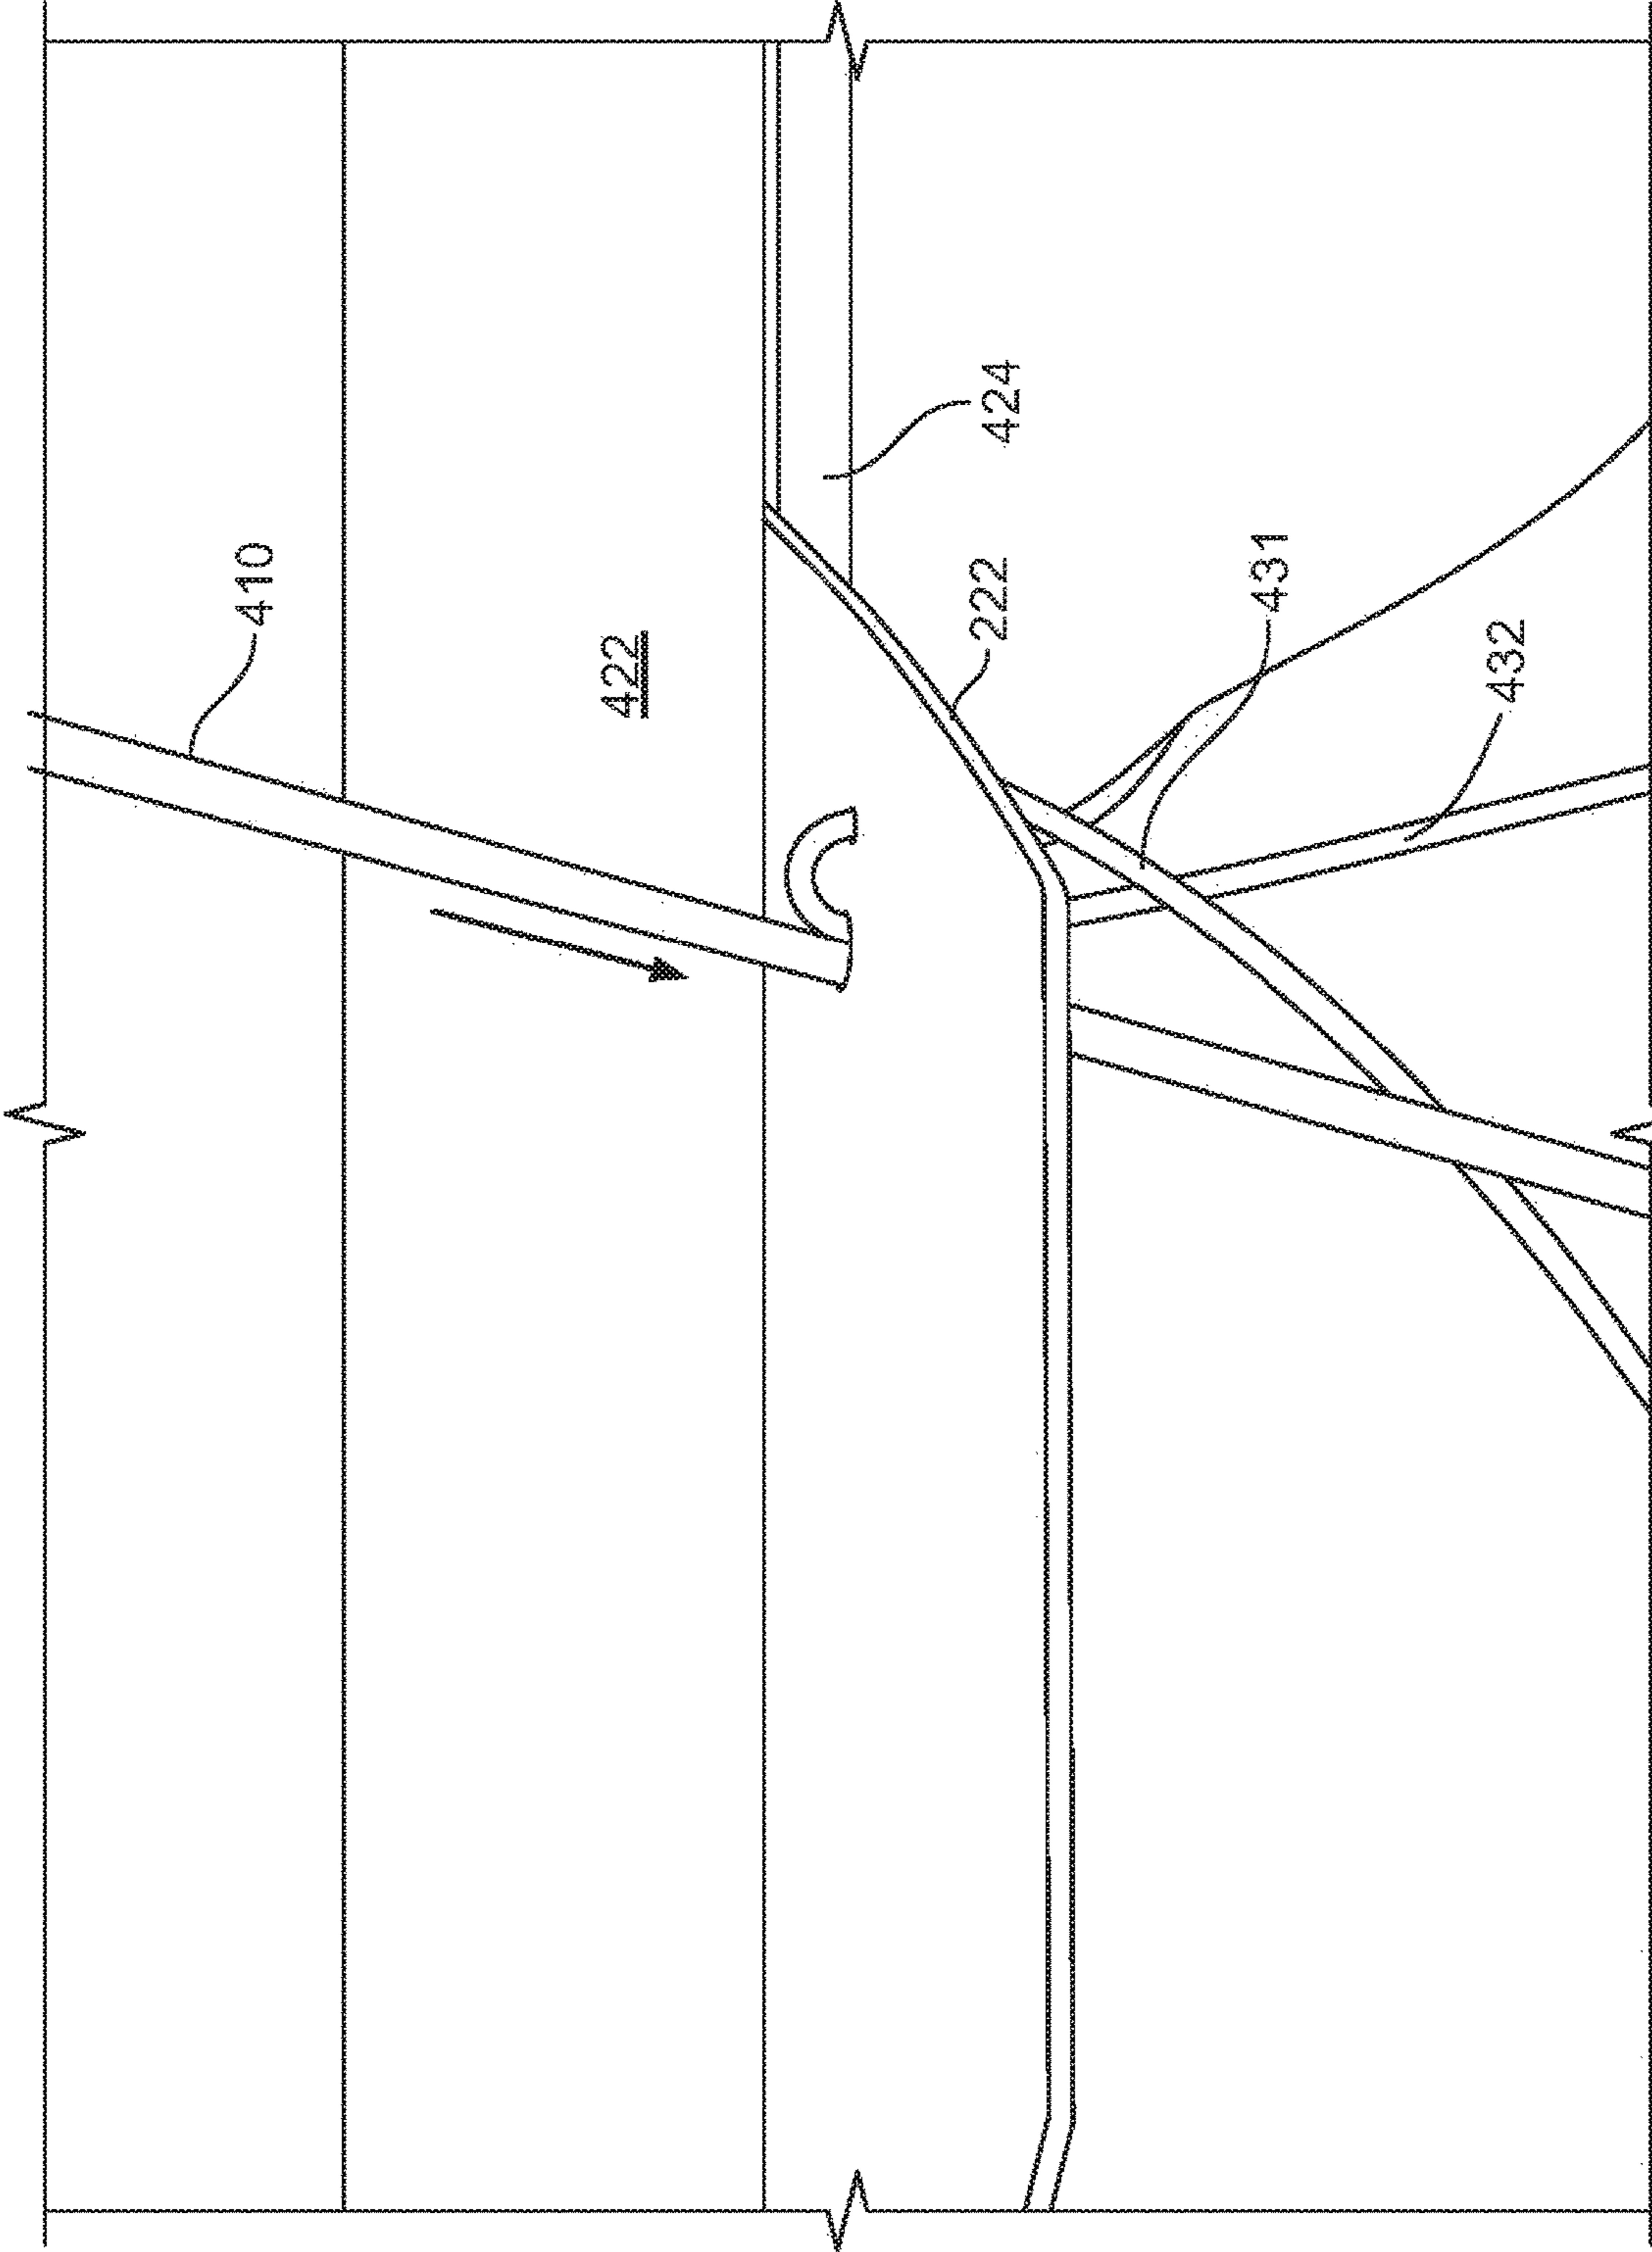


FIG. 4C

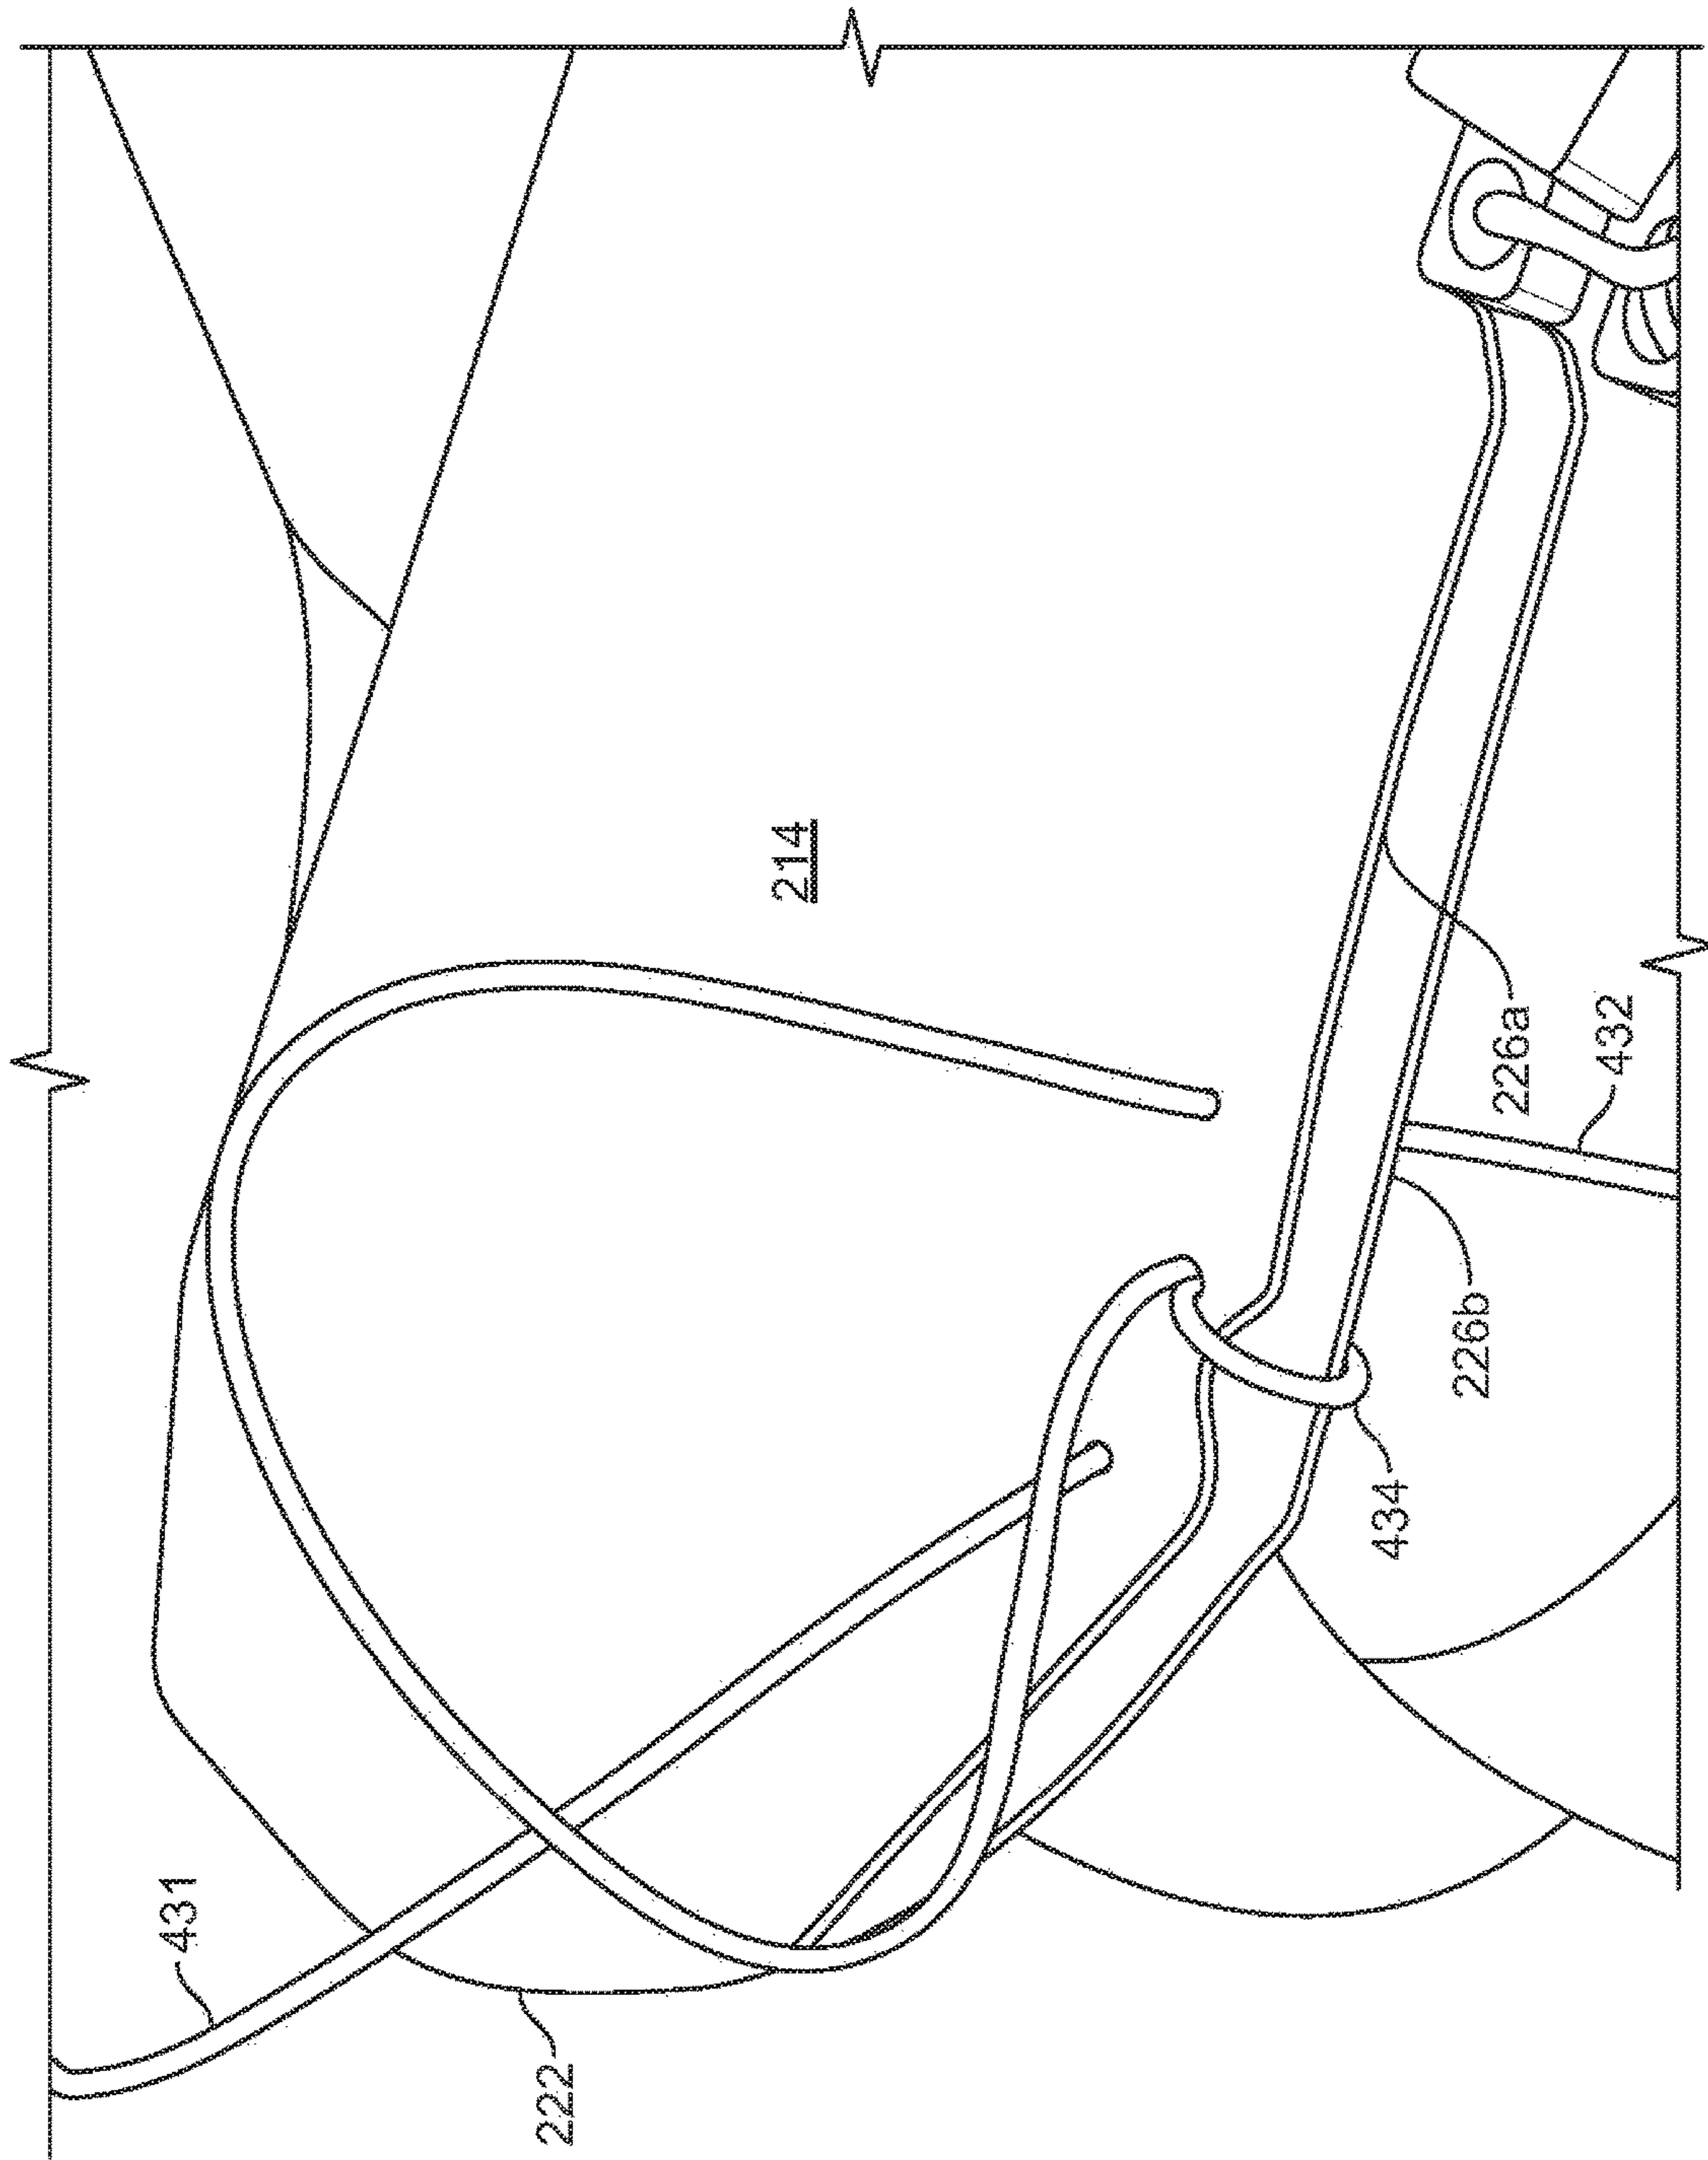


FIG. 4D

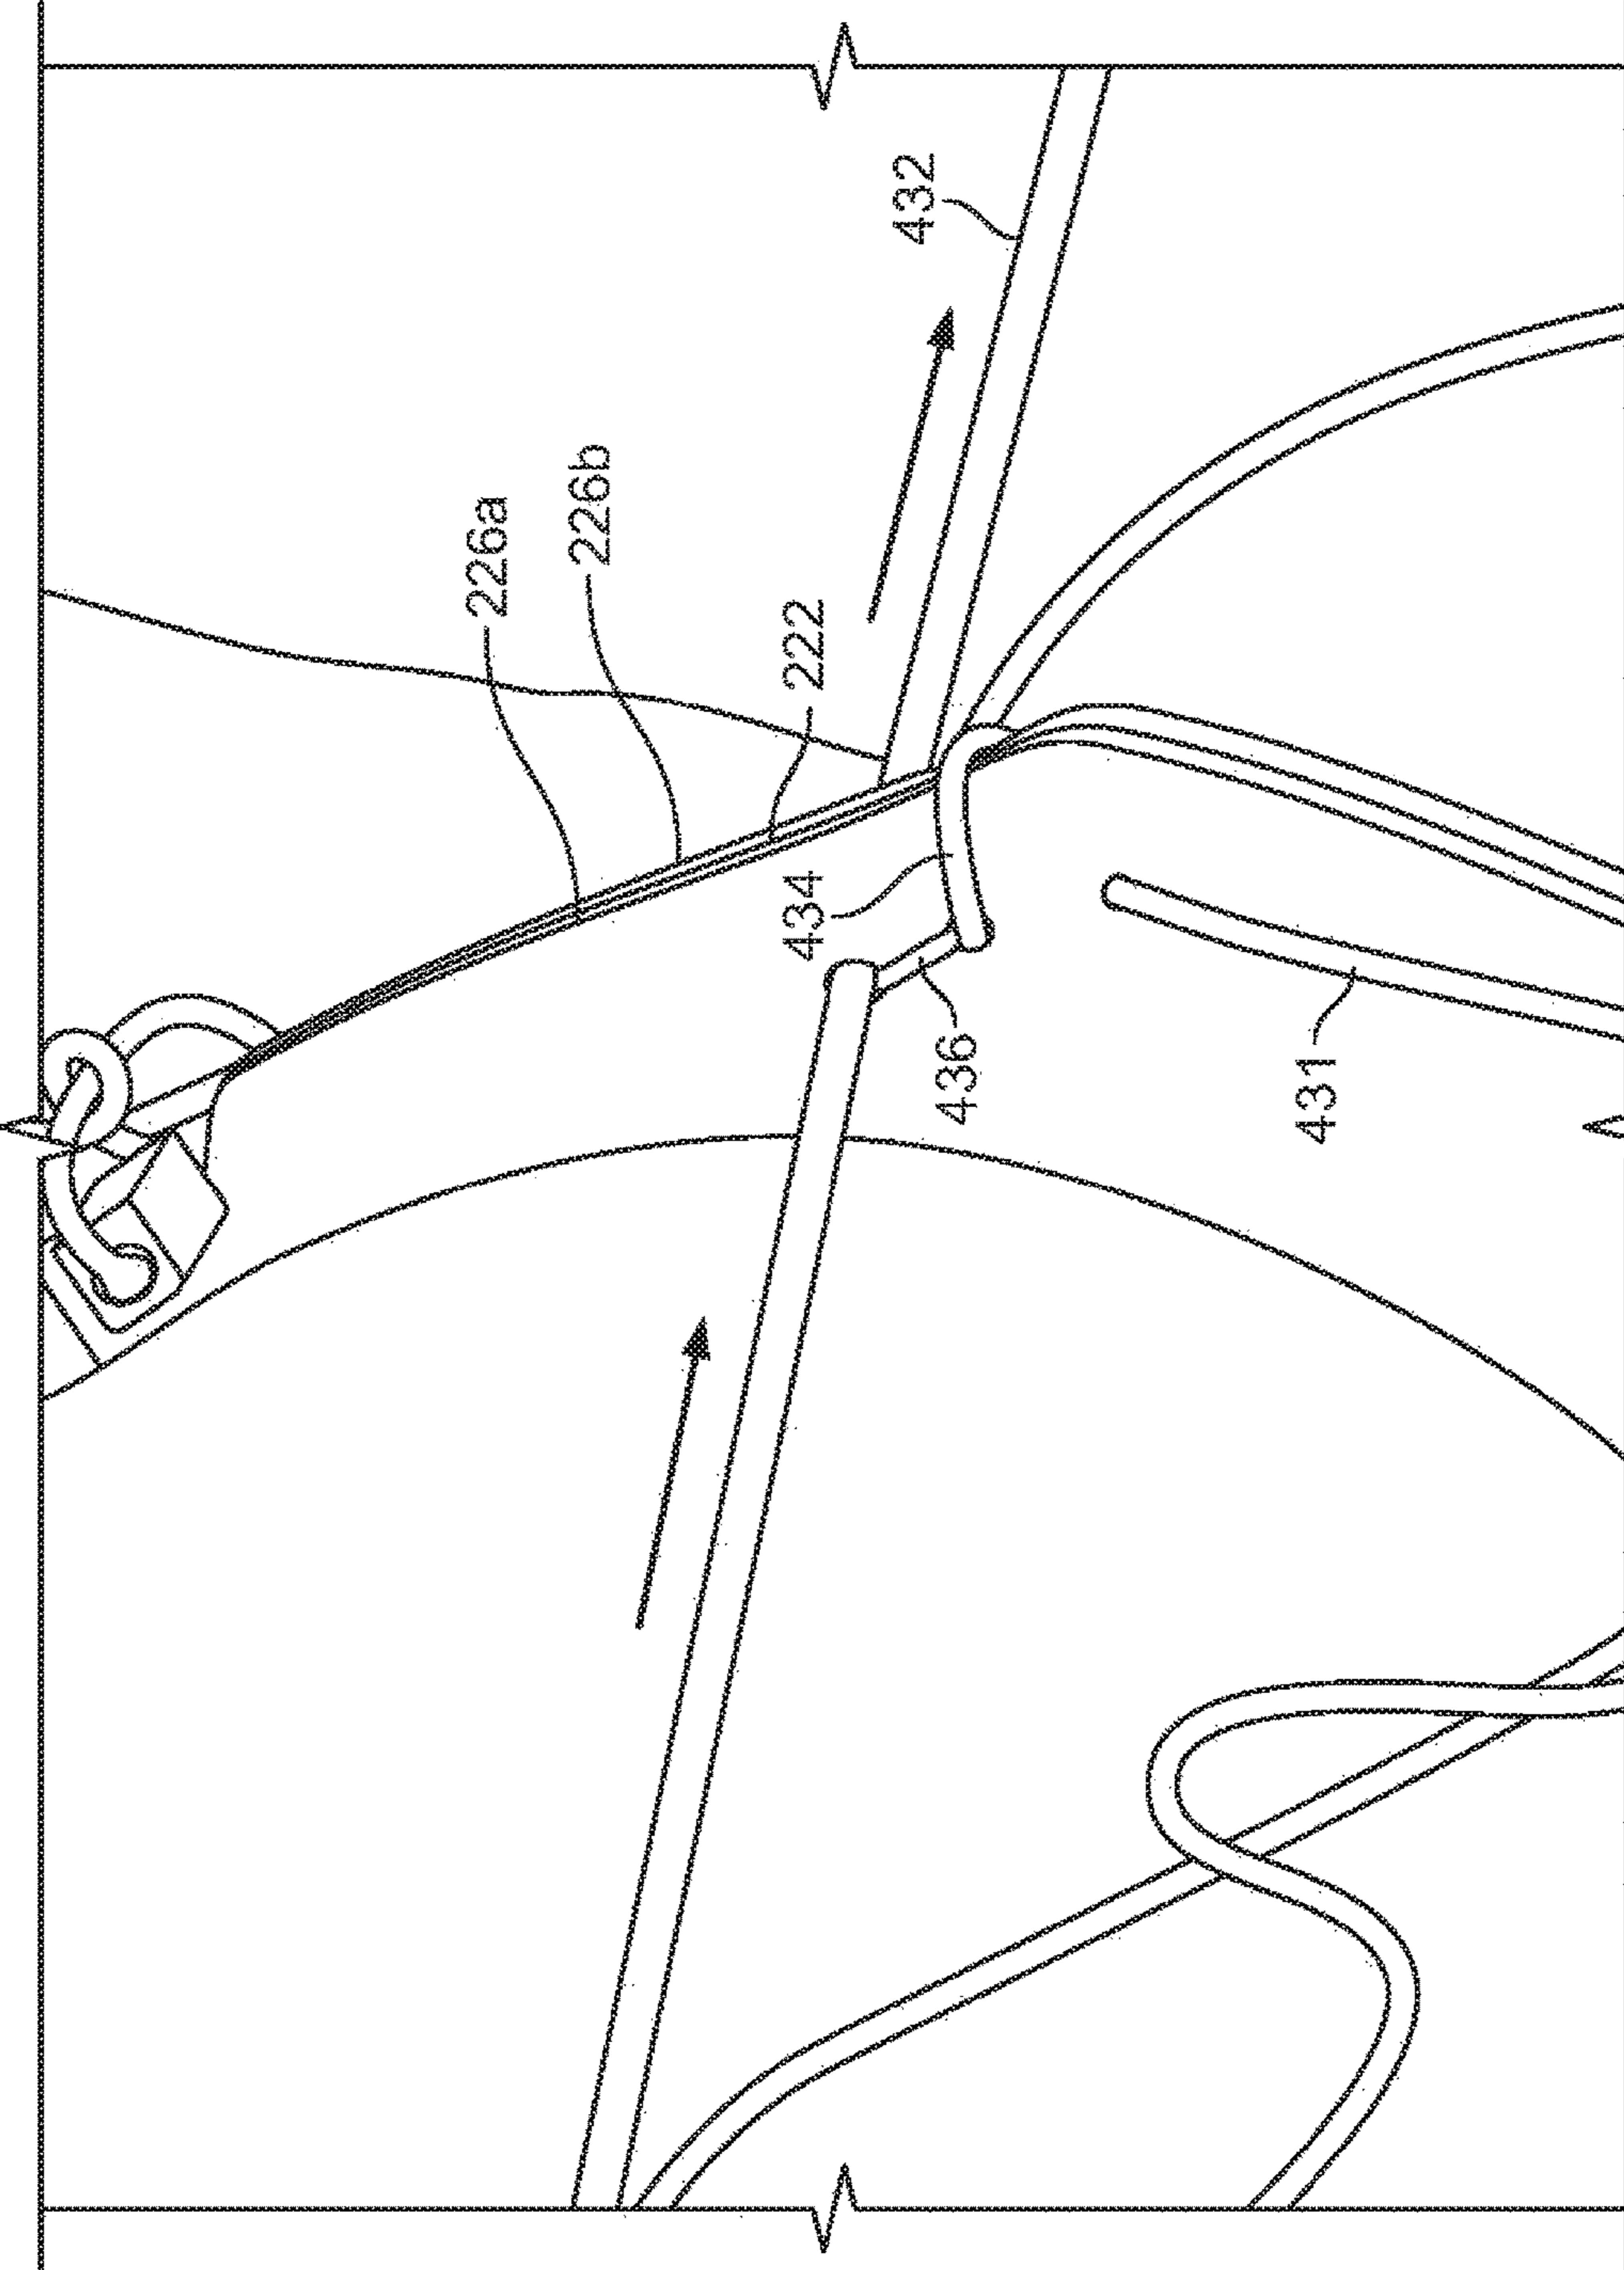


FIG. 4E

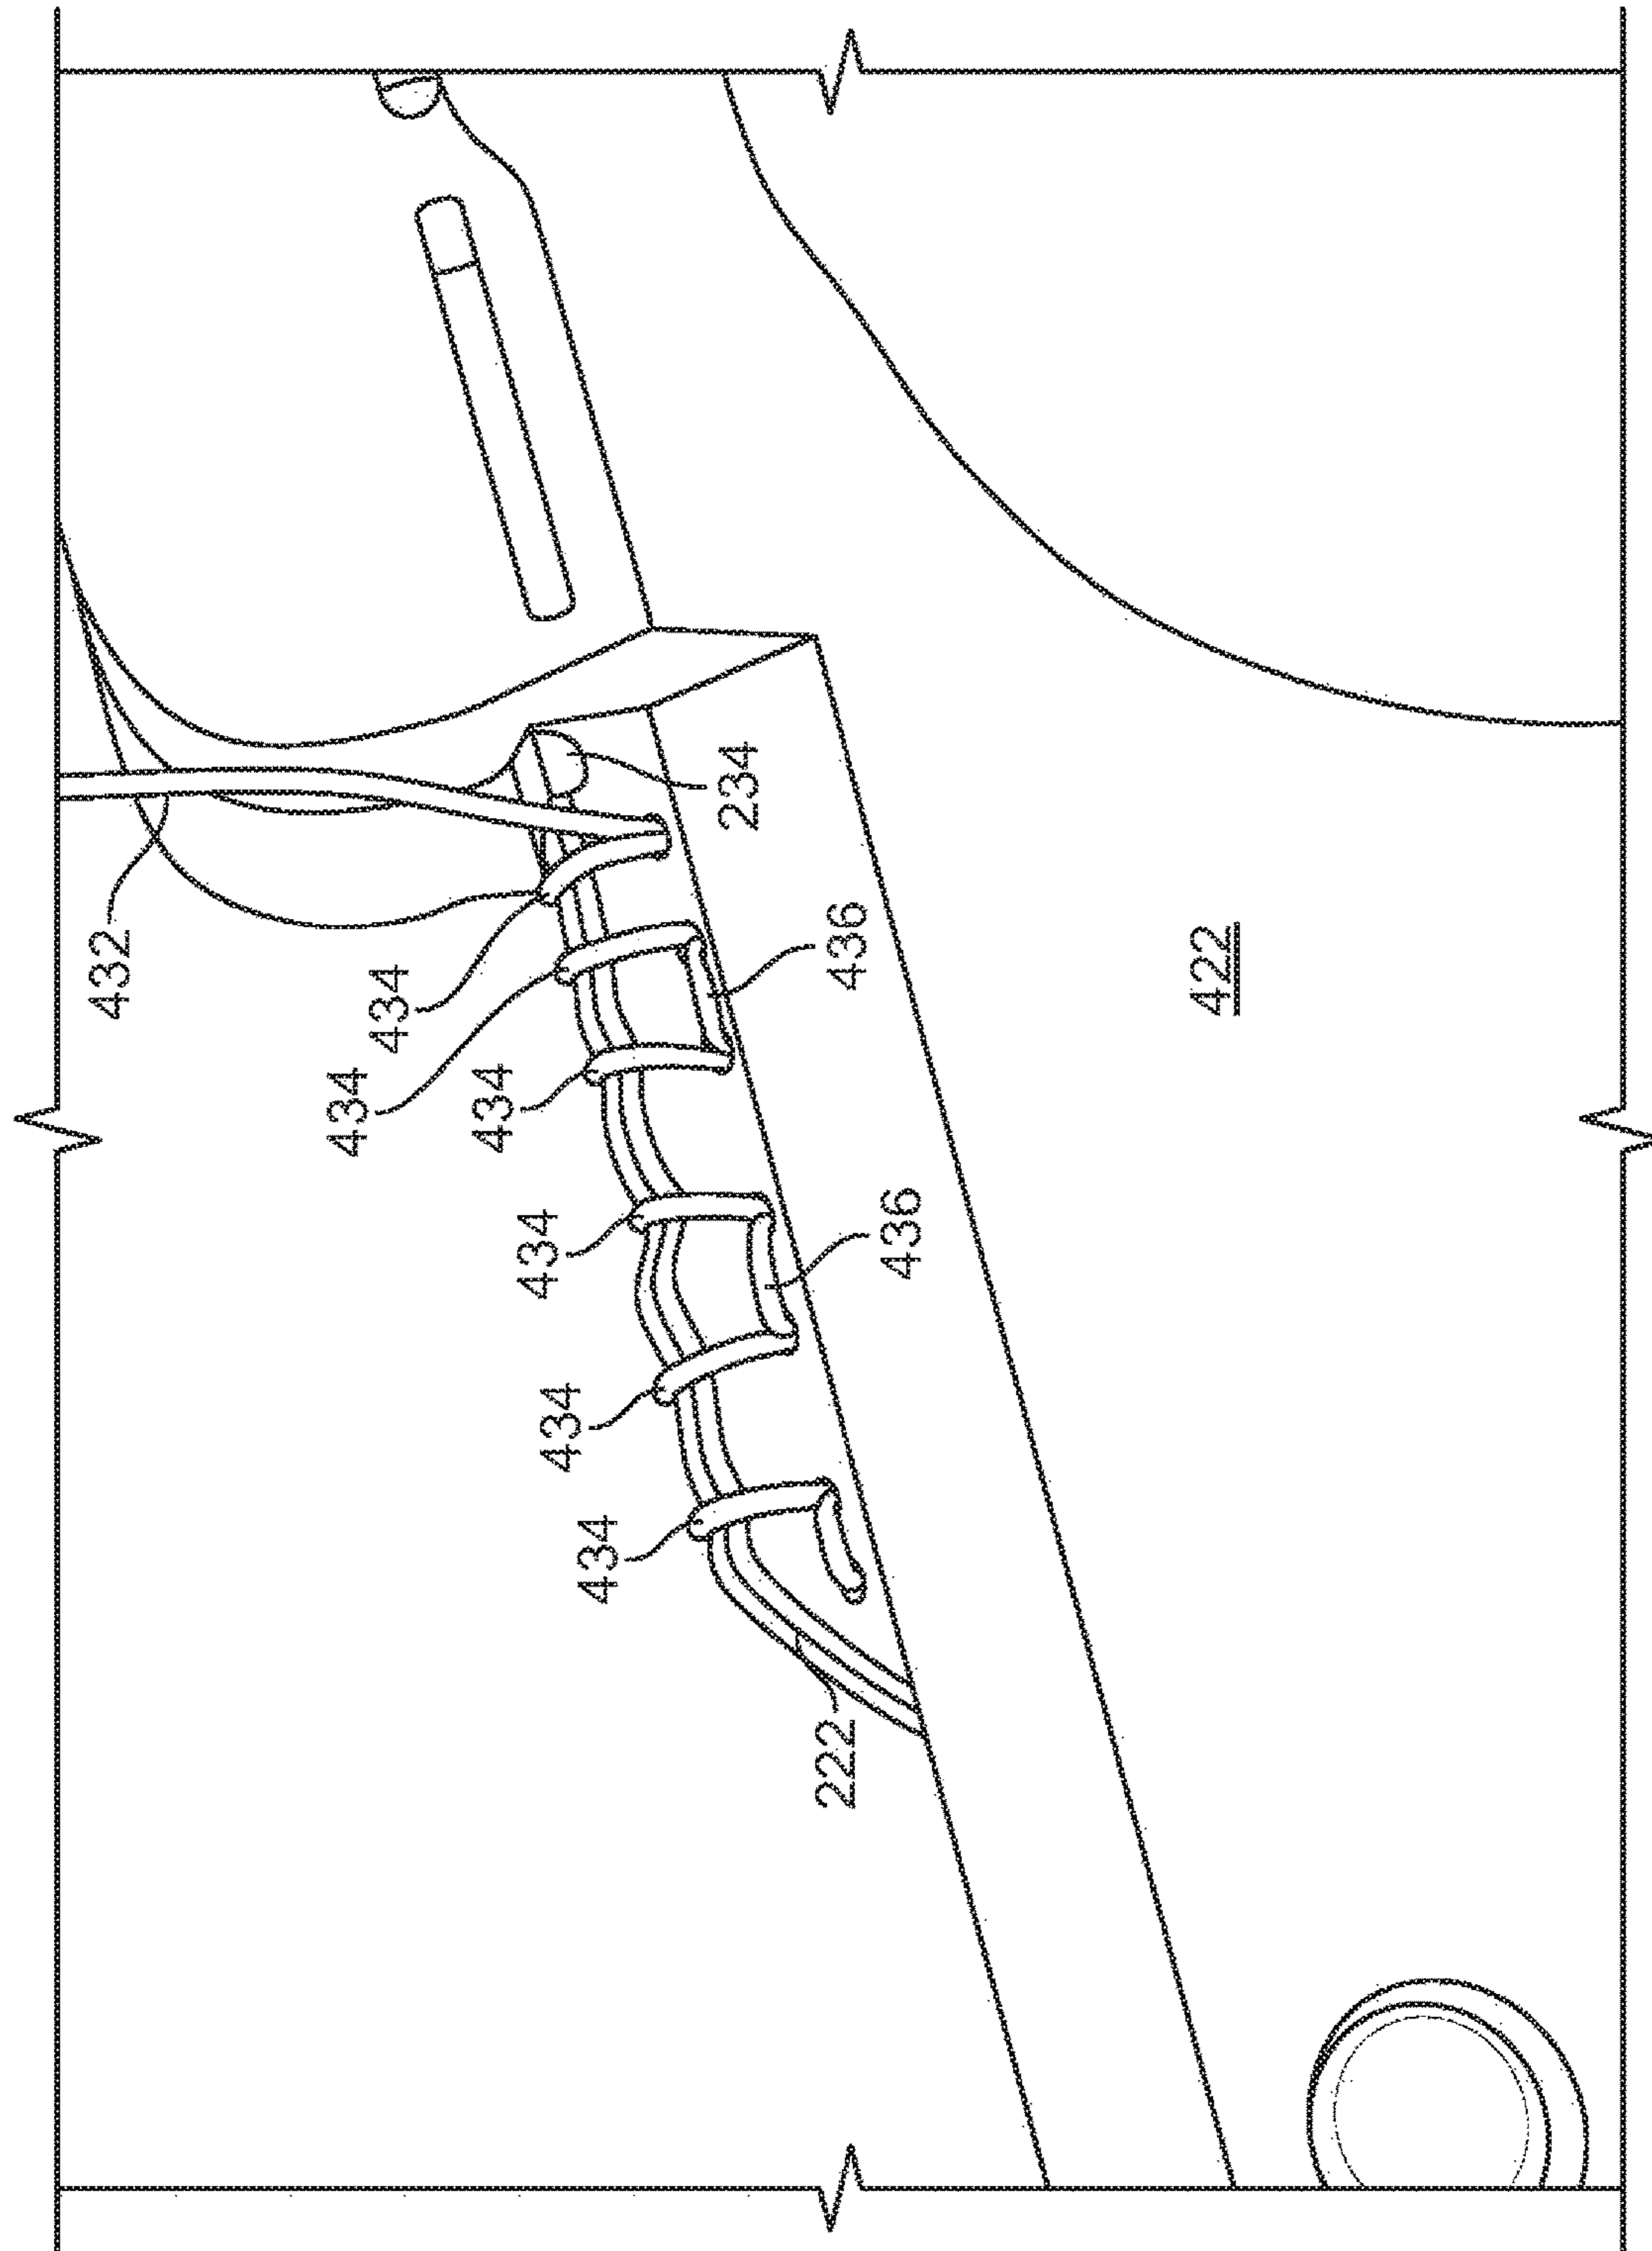


FIG. 4F

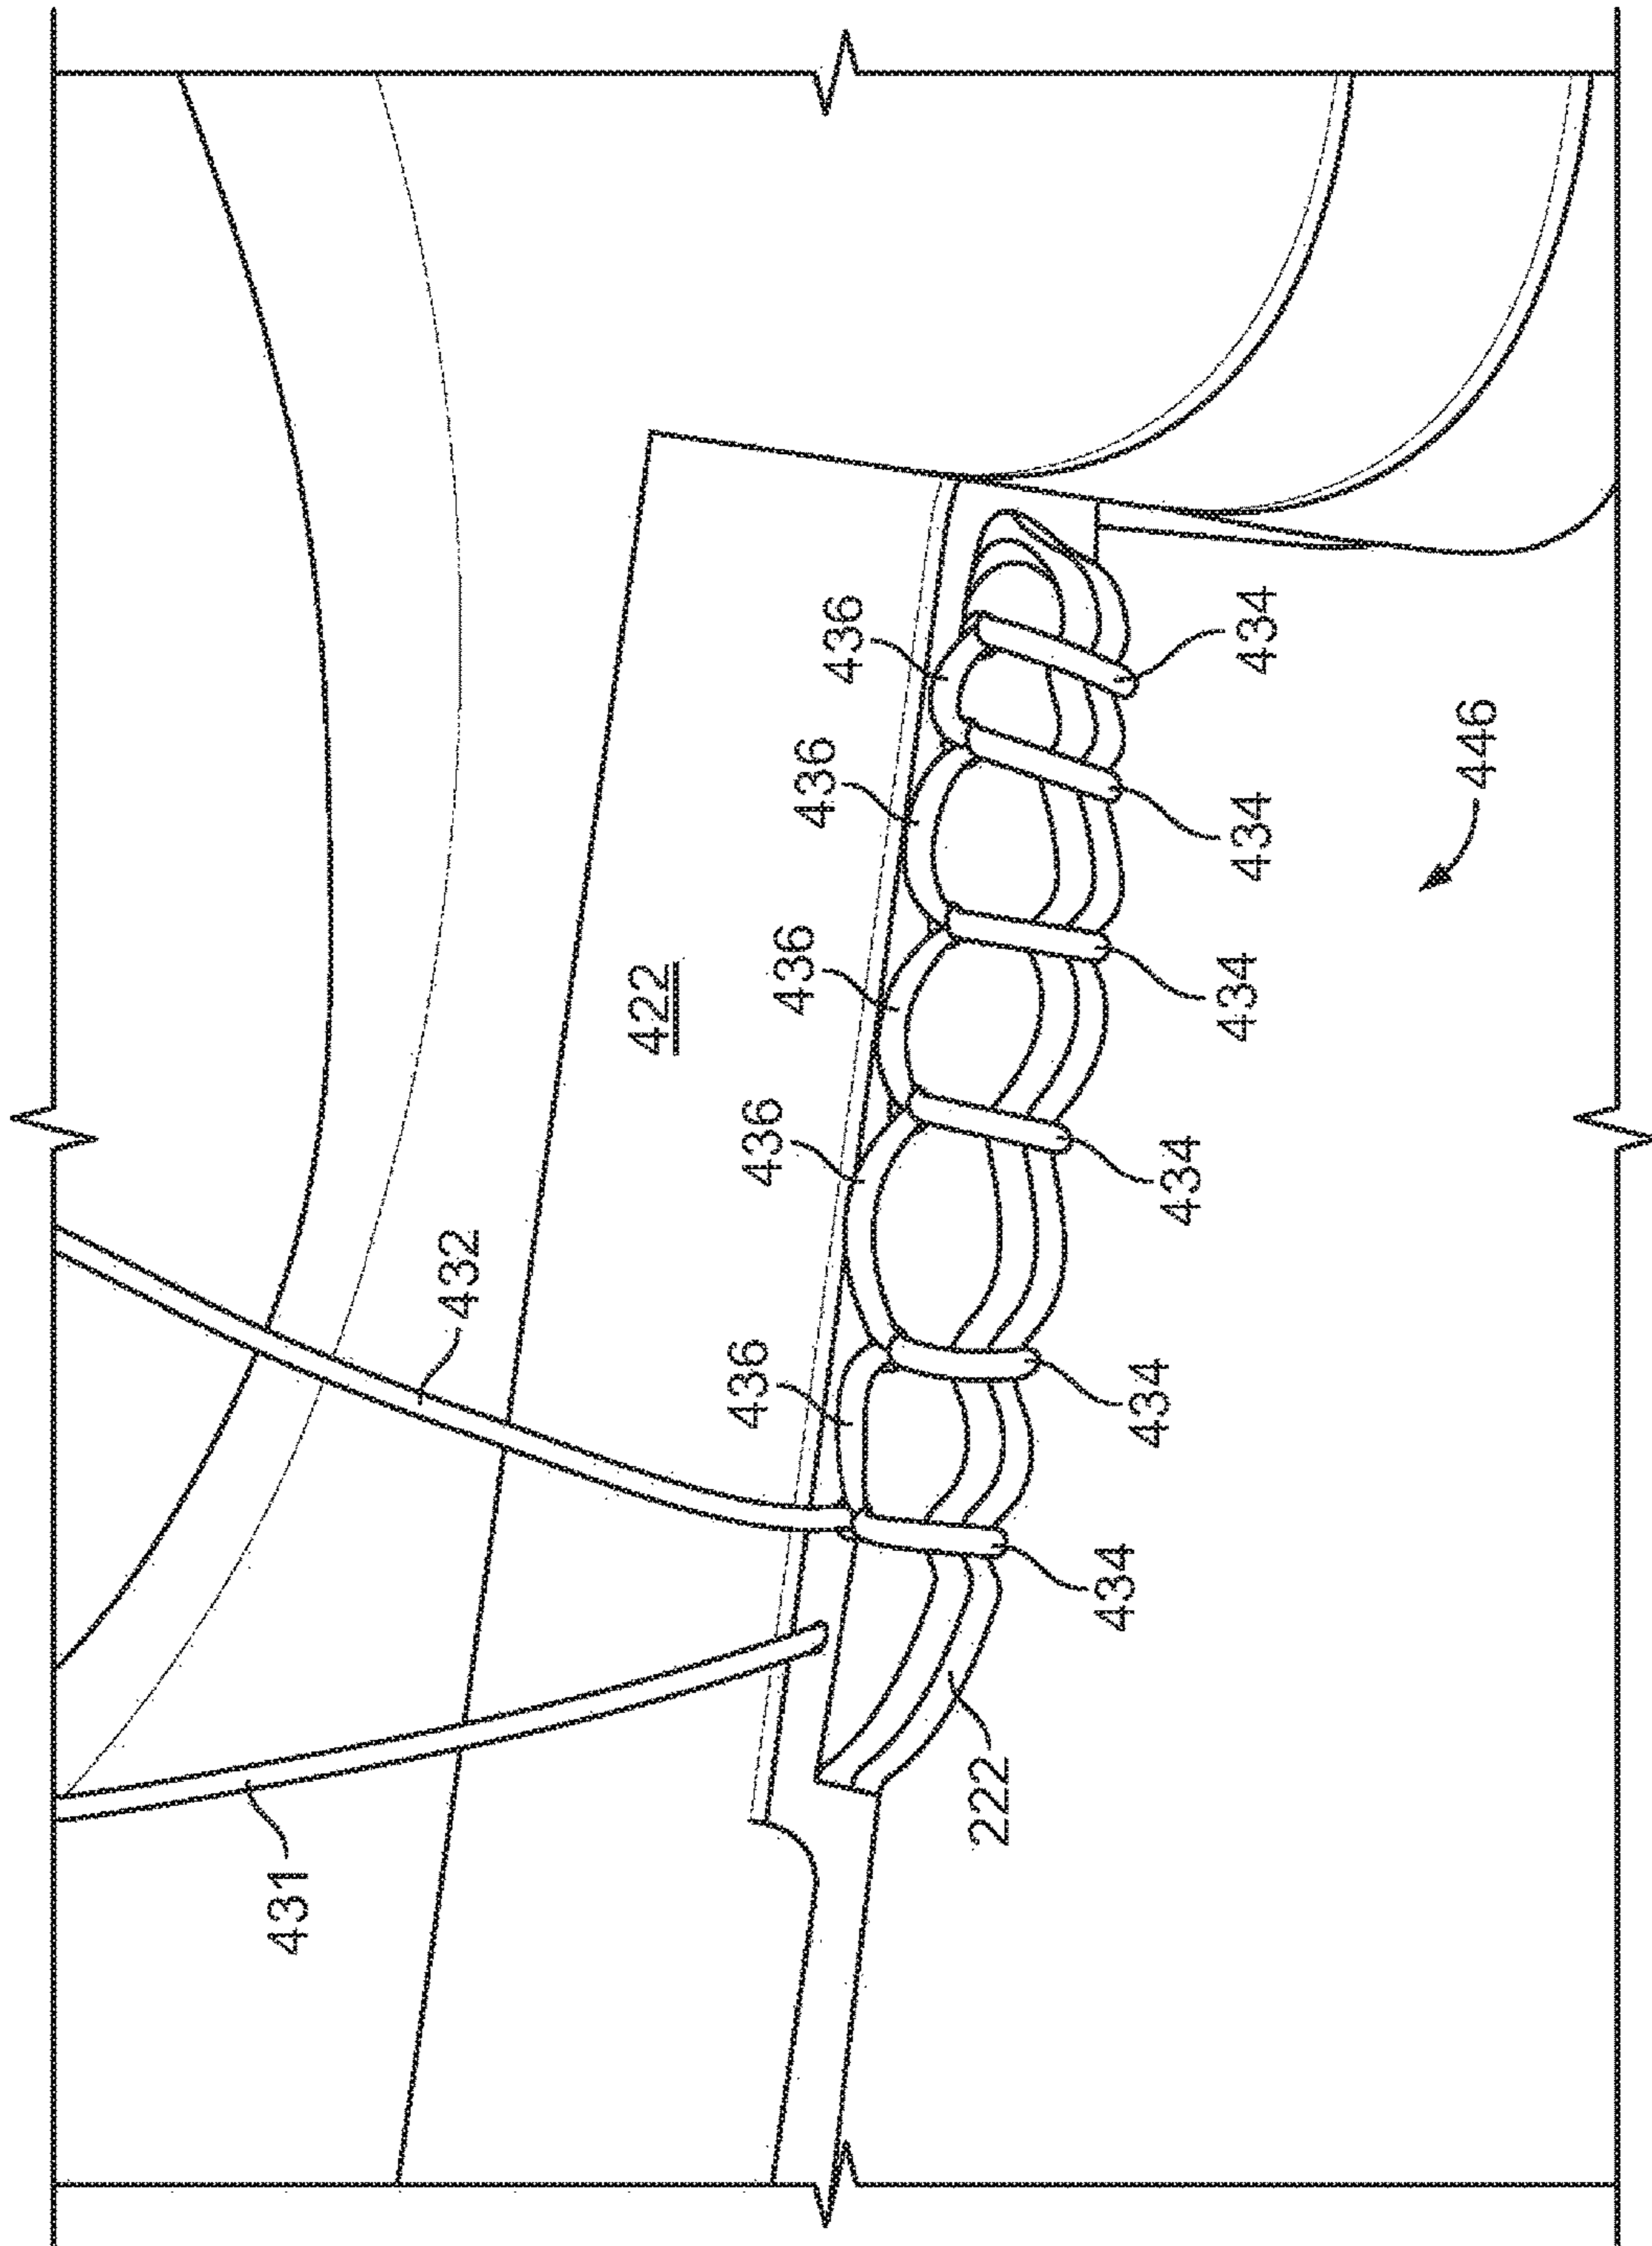


FIG. 4G

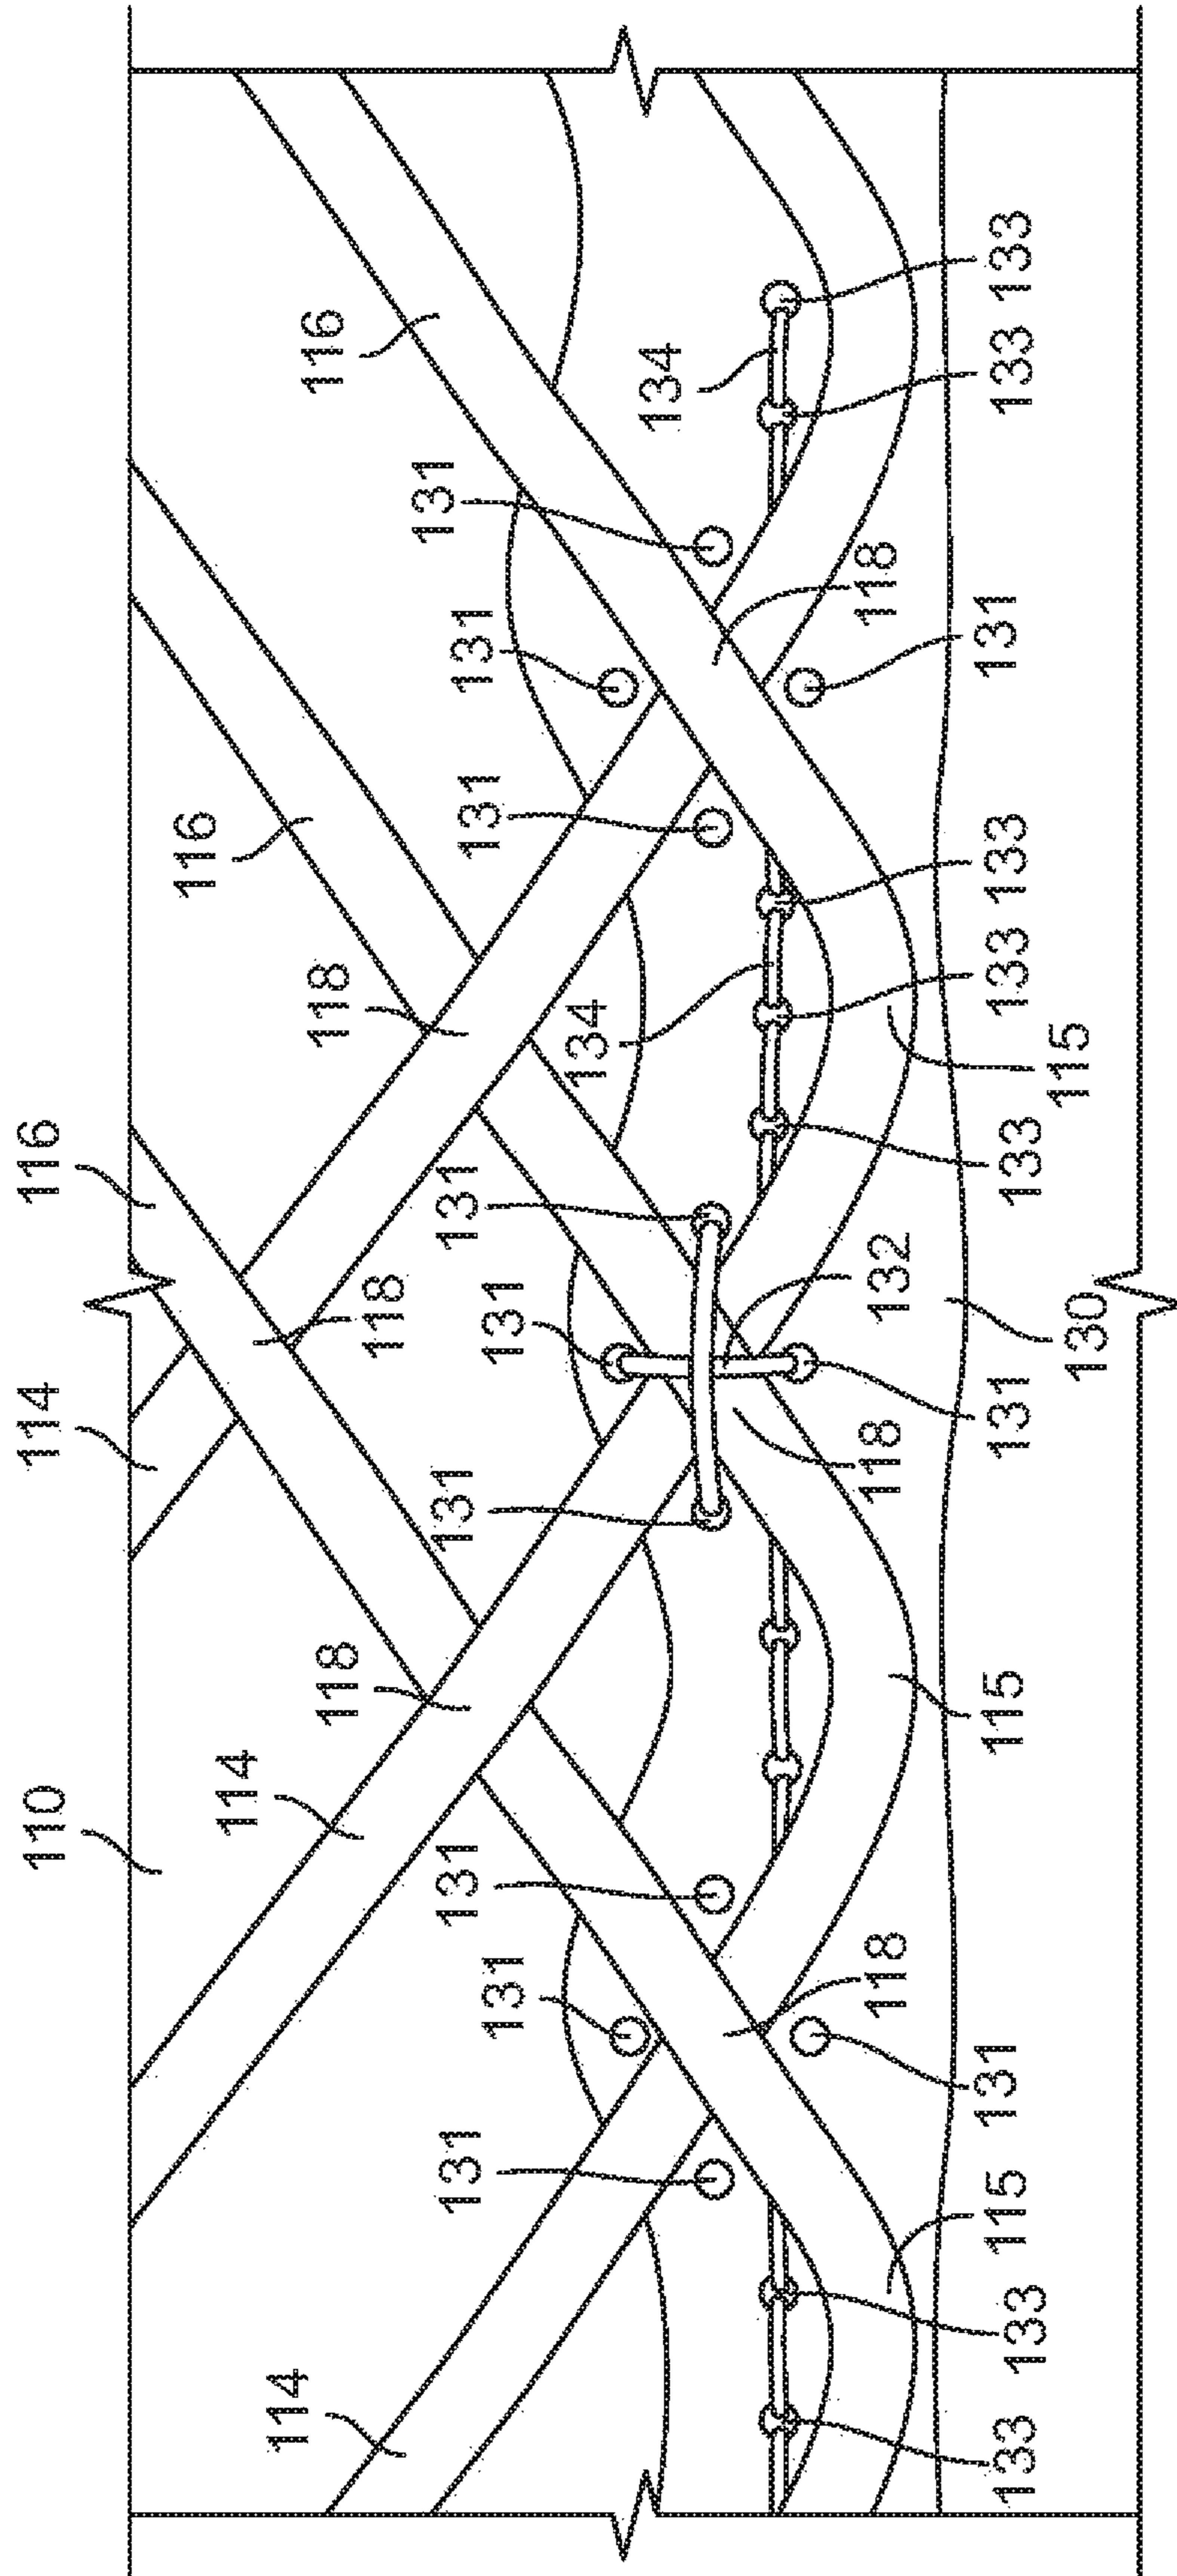


FIG. 5A

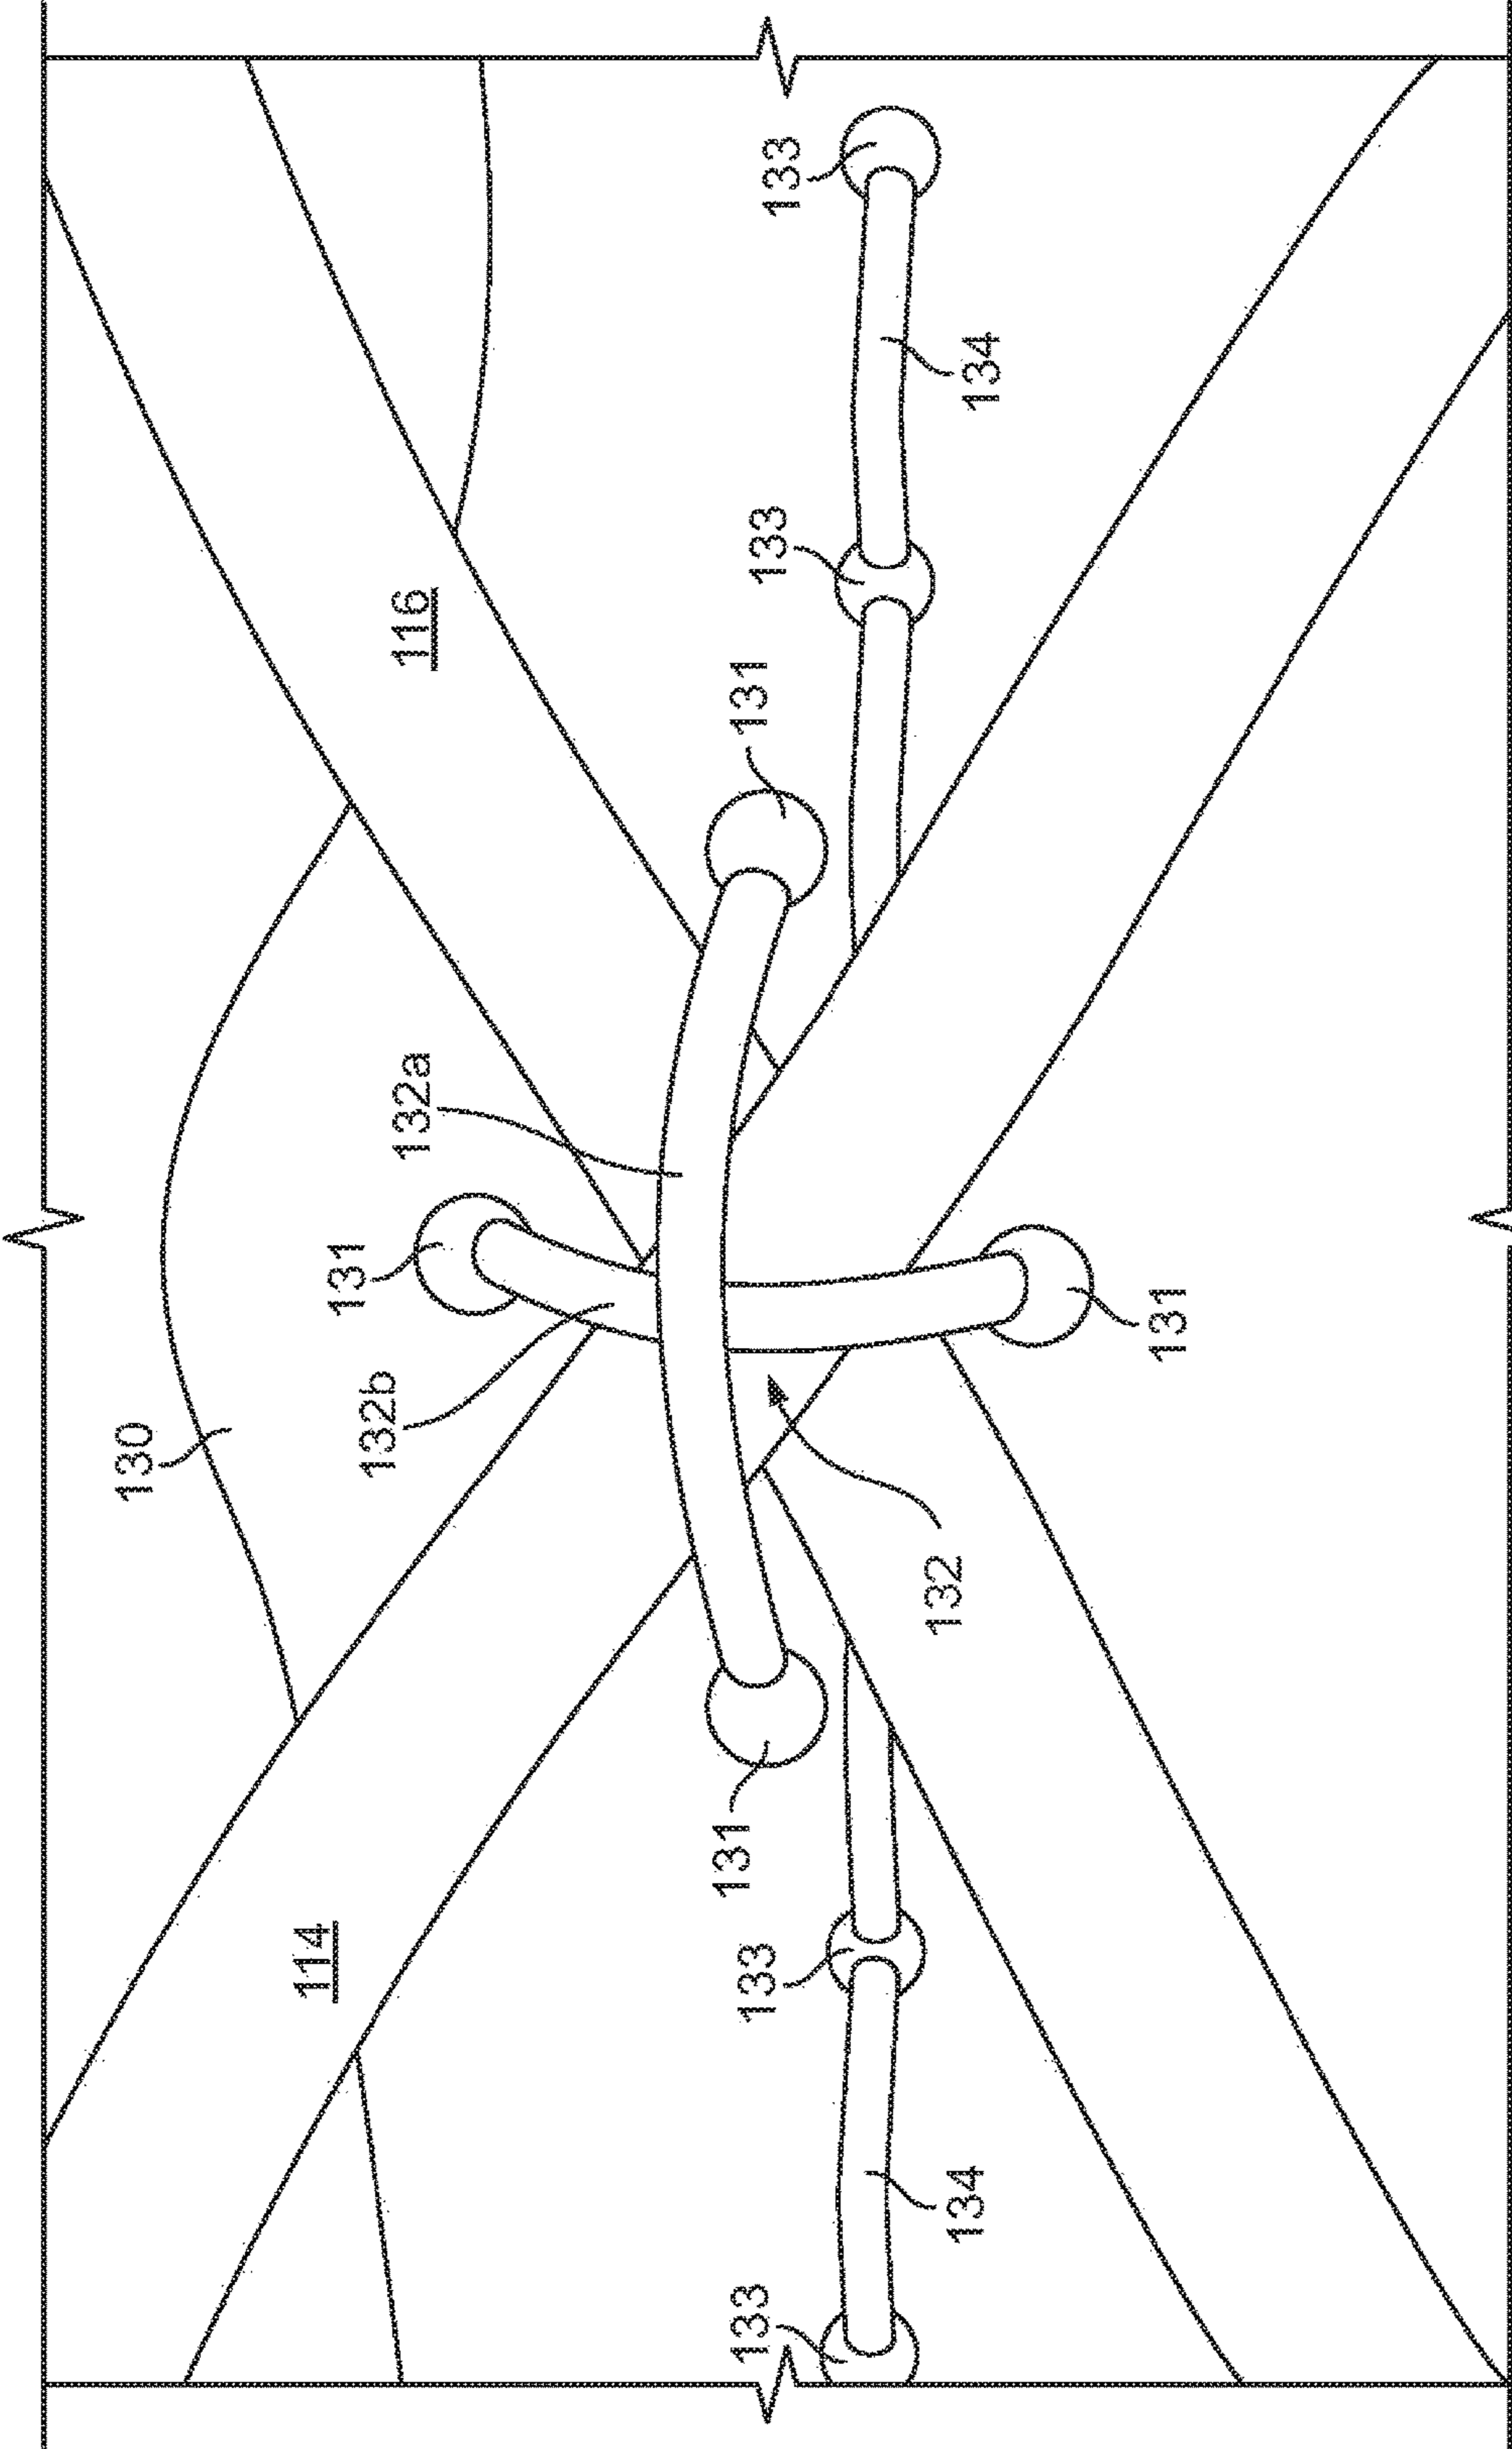


FIG. 5B

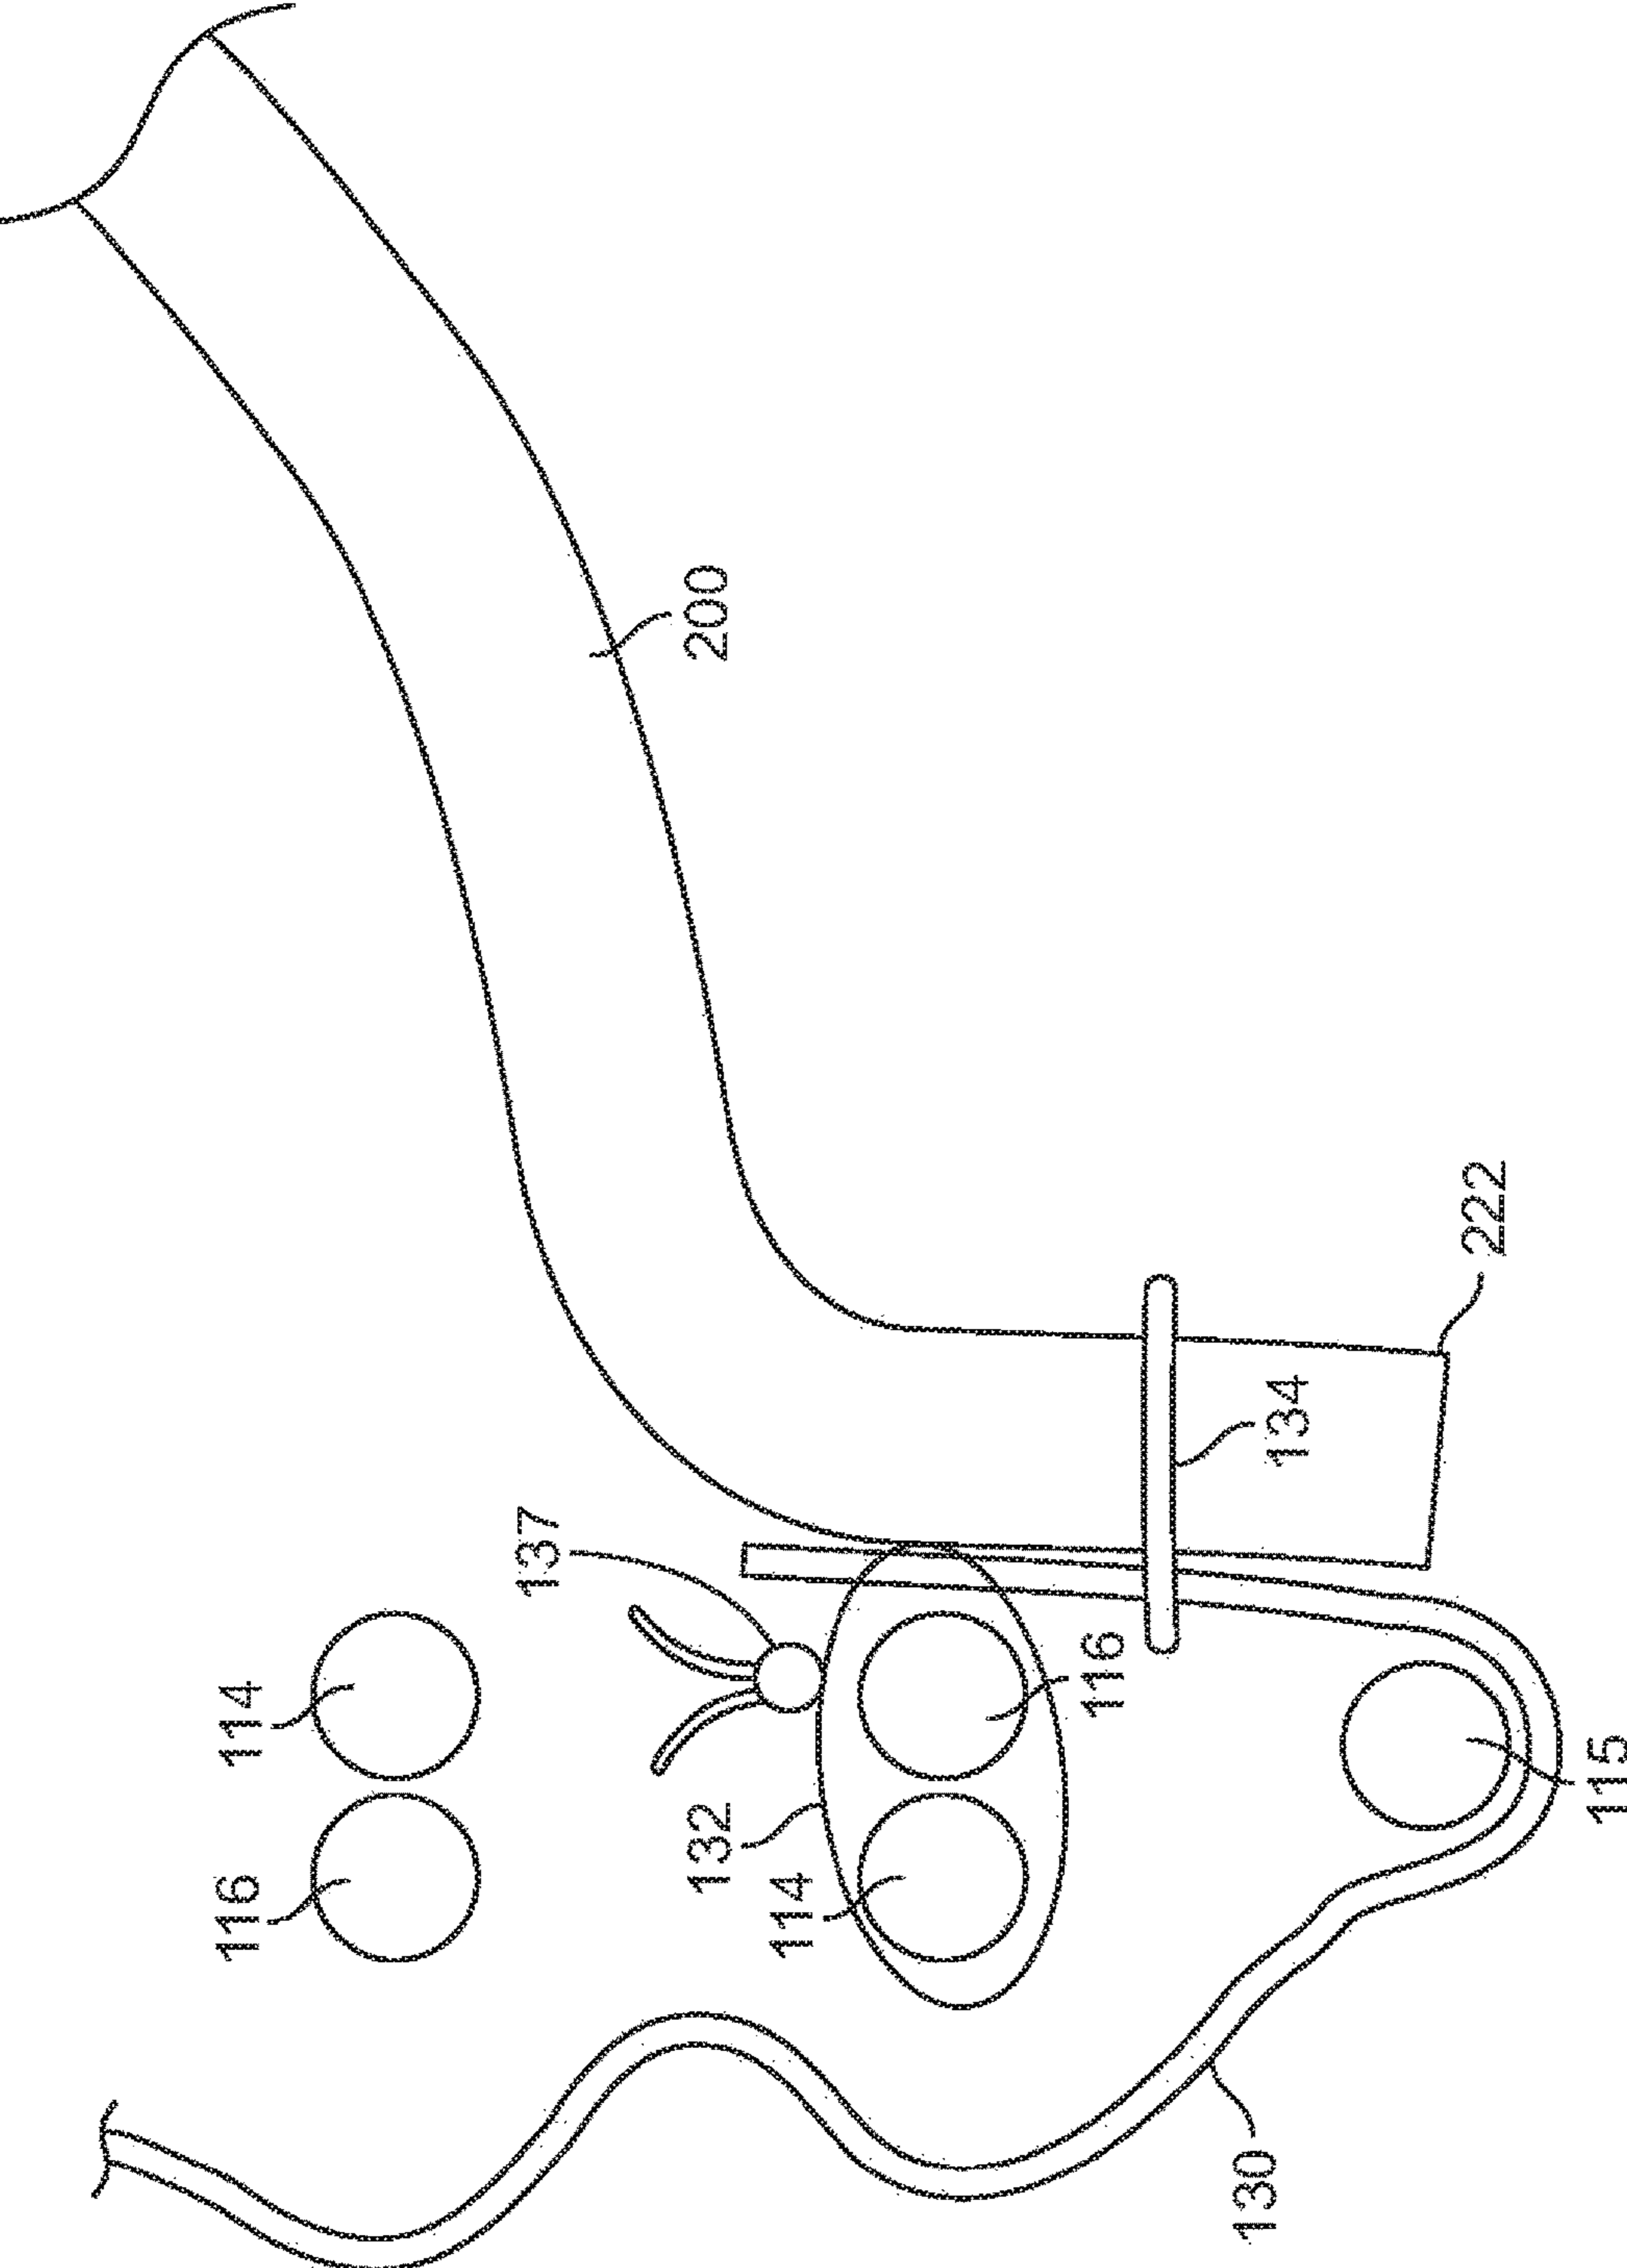


FIG. 5C

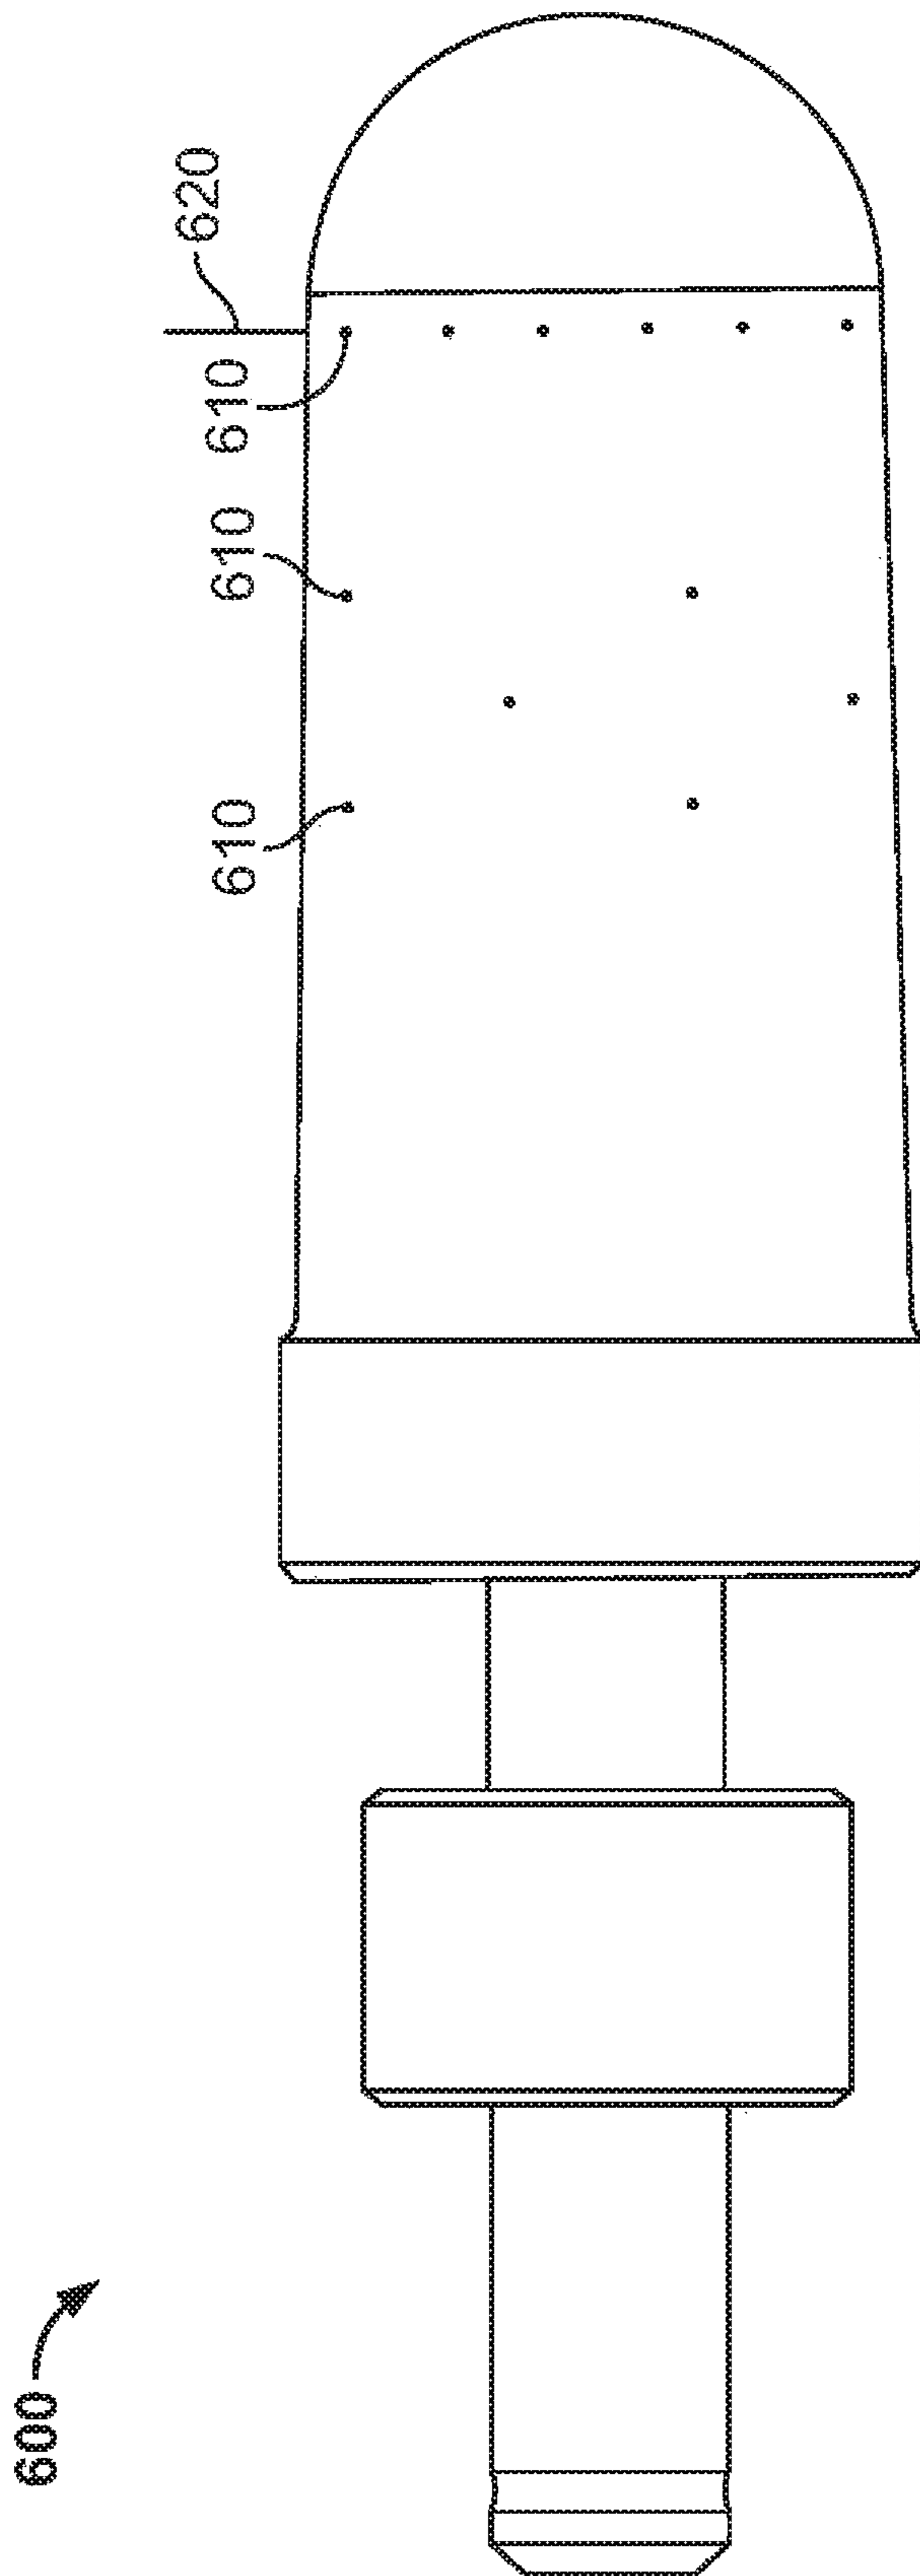


FIG. 6

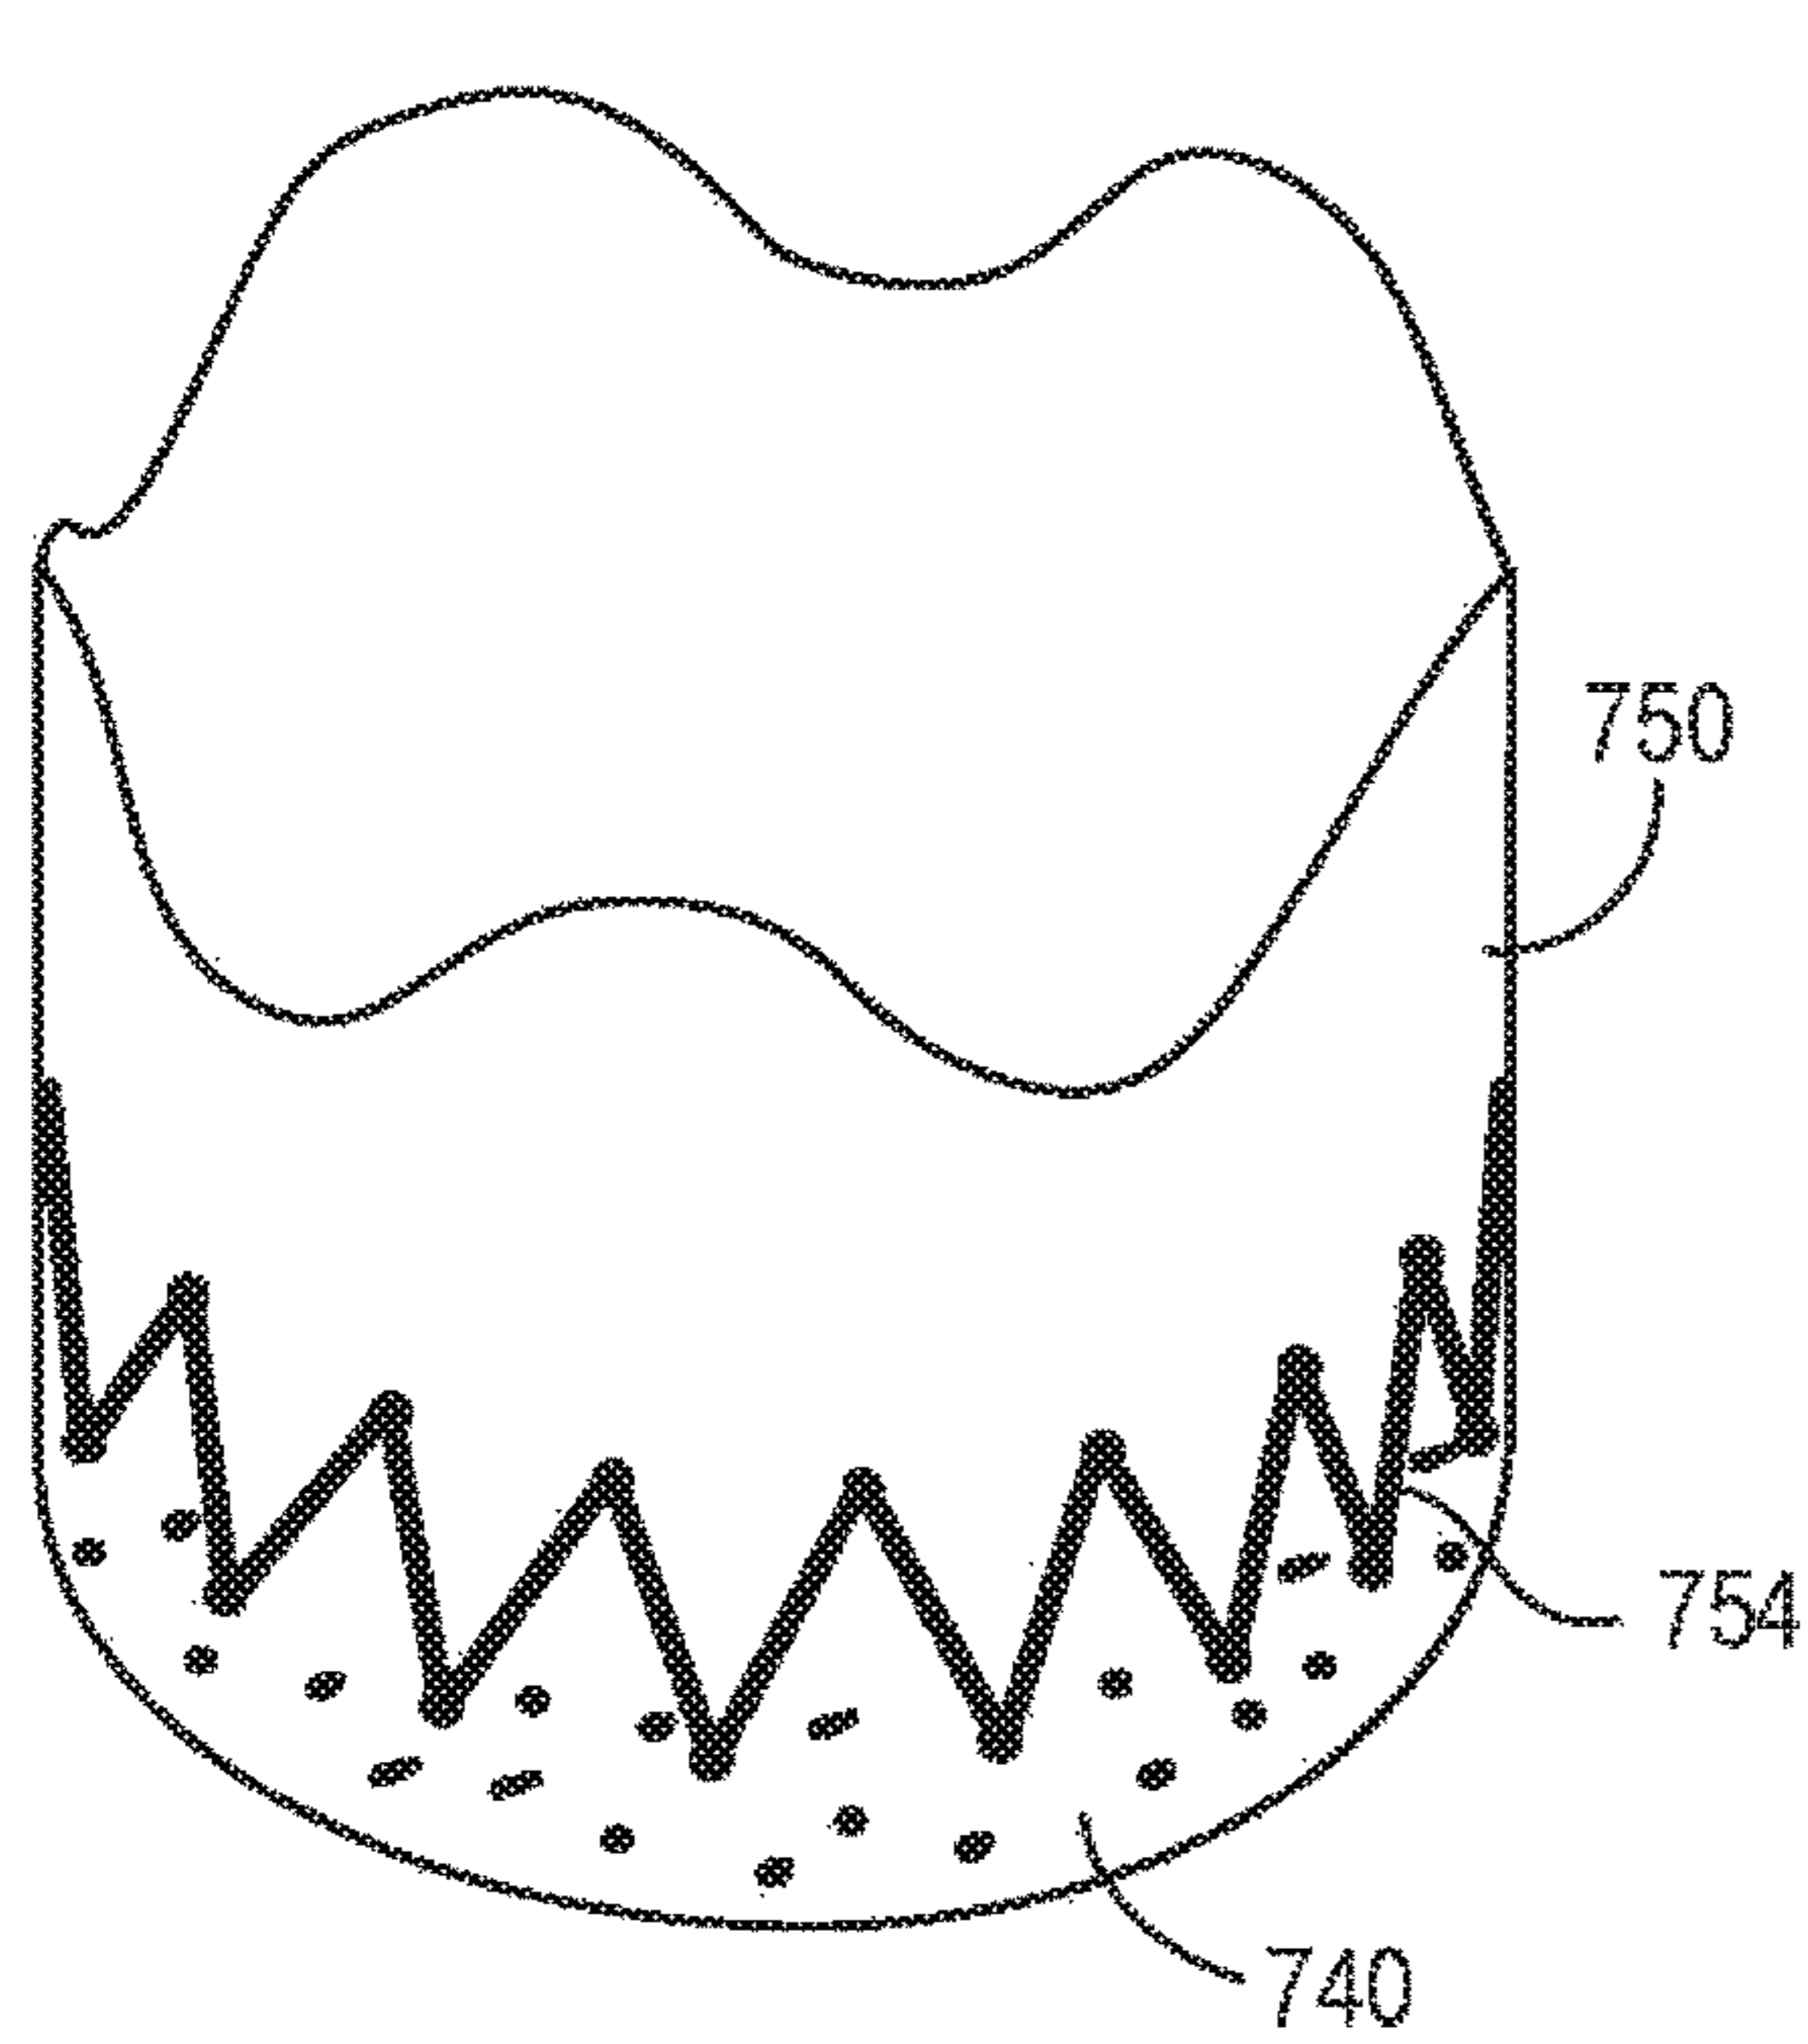
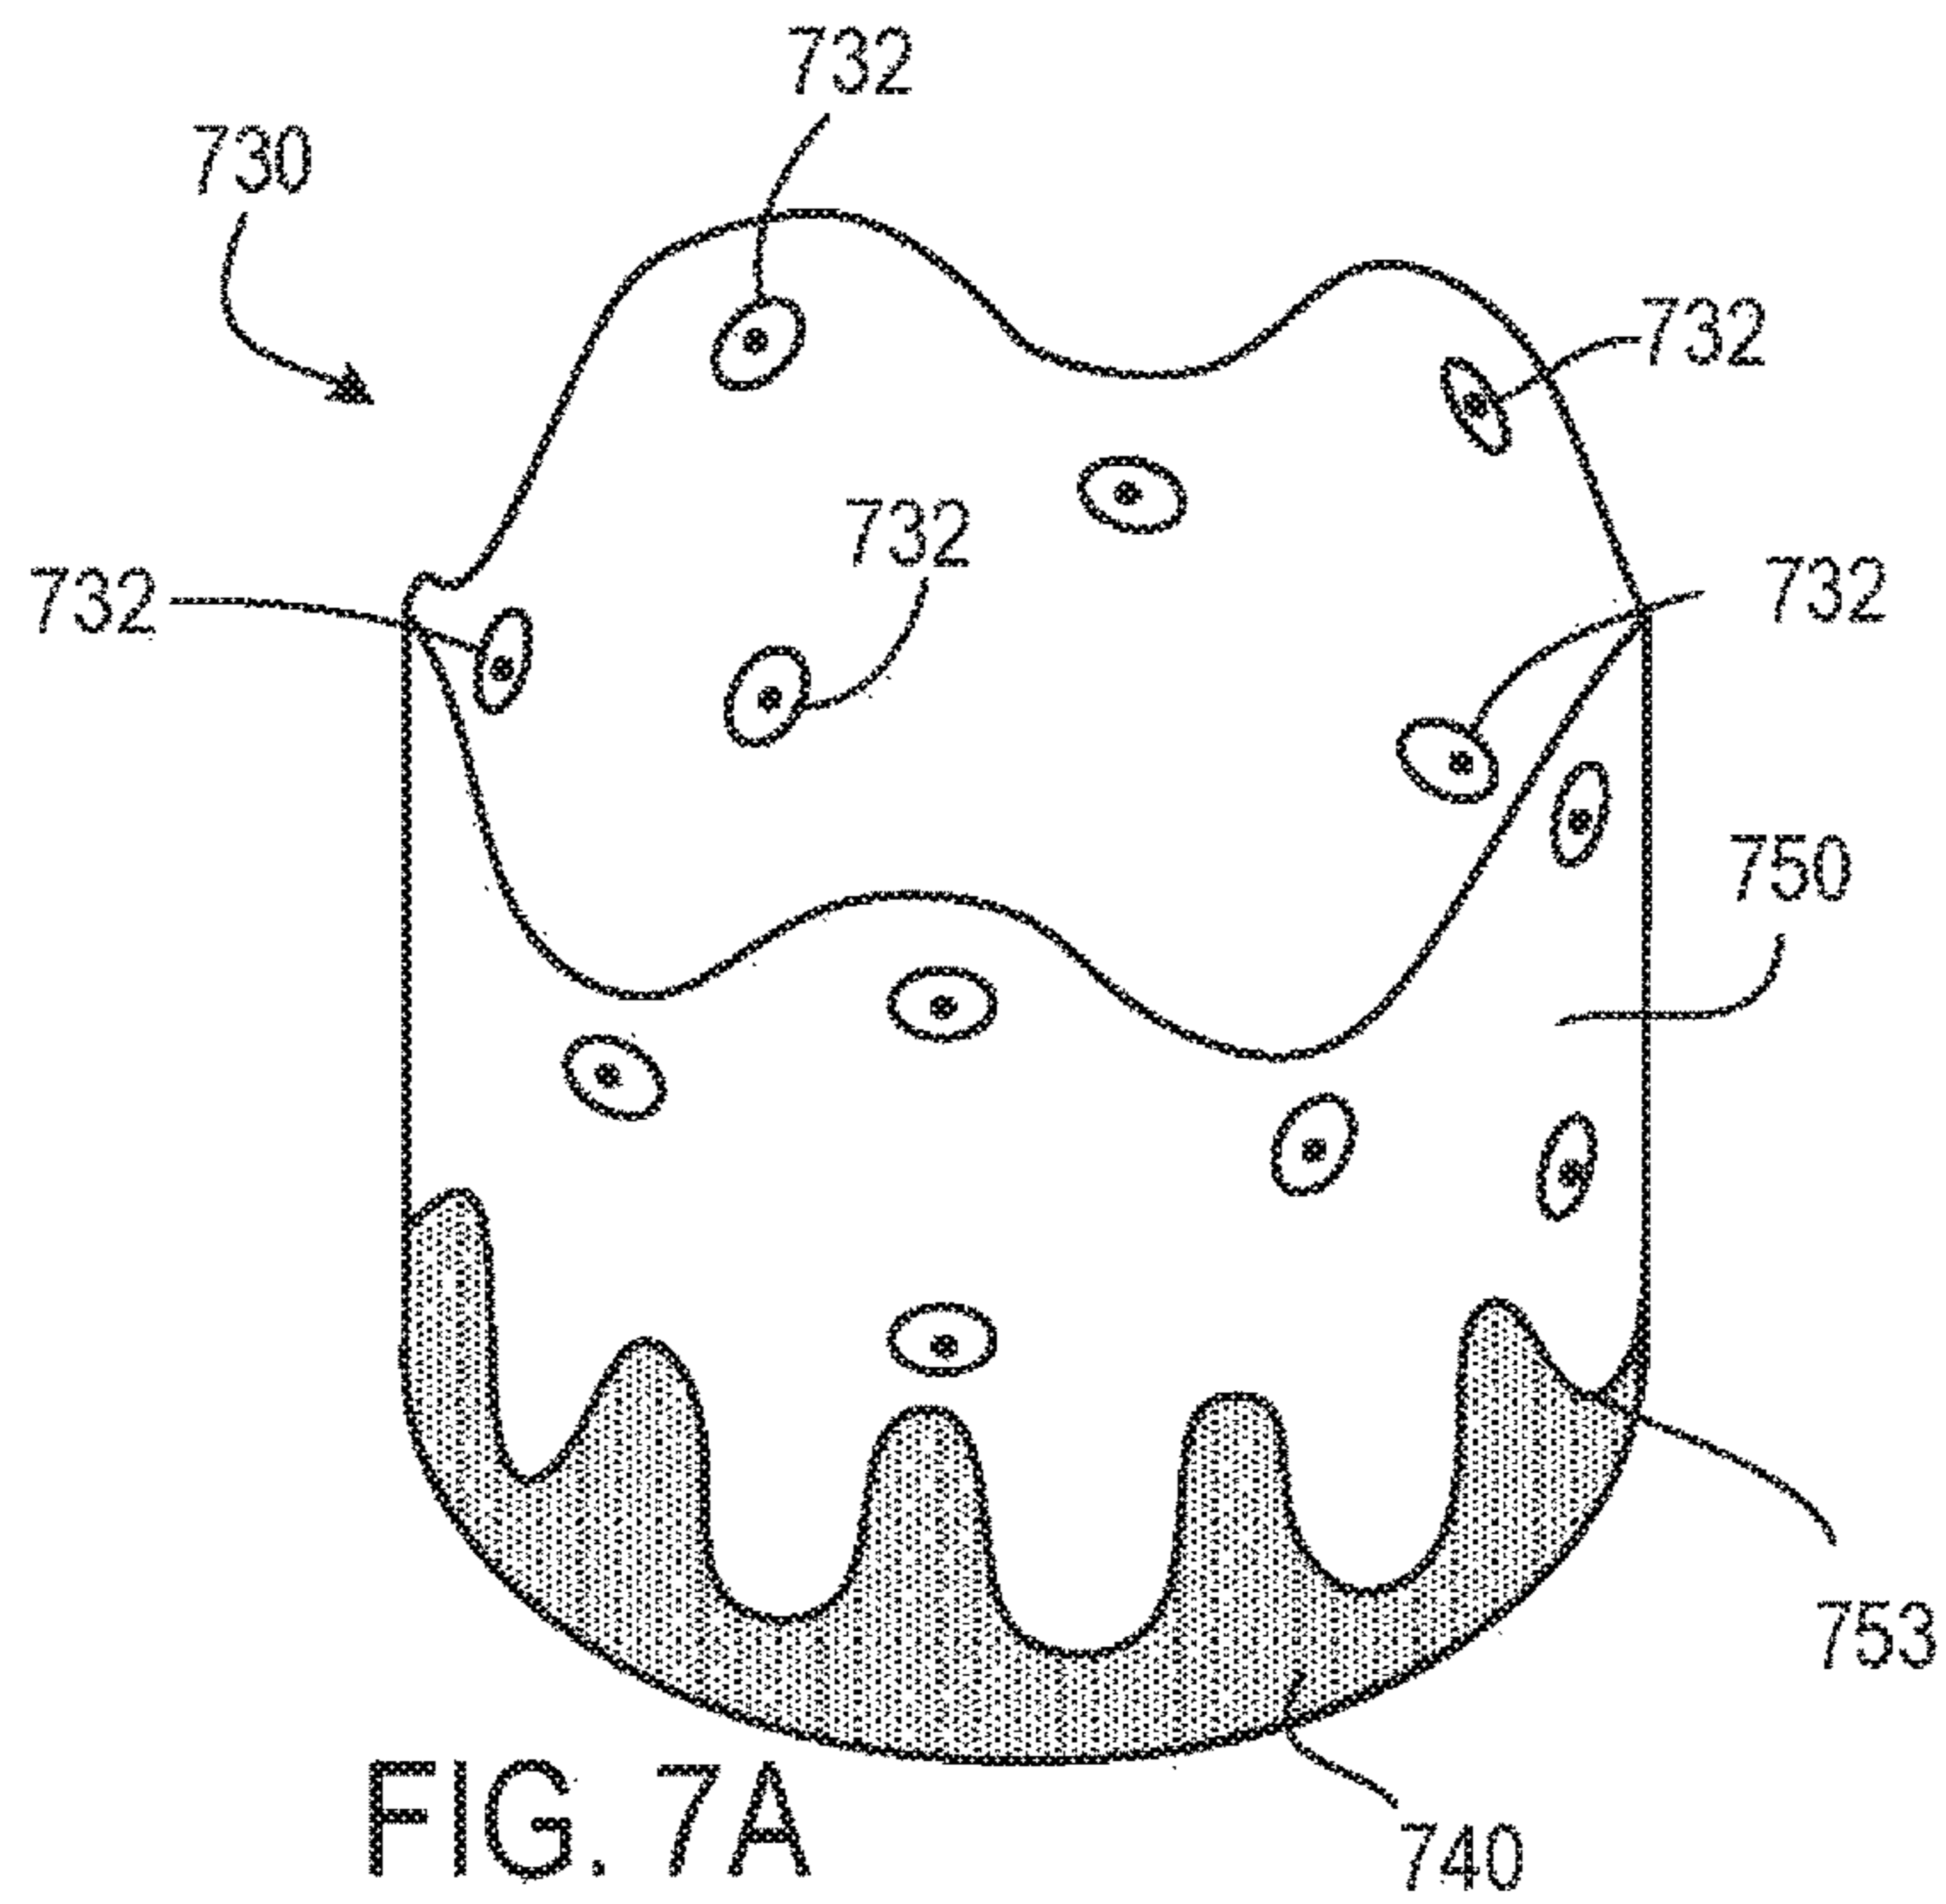


FIG. 7B

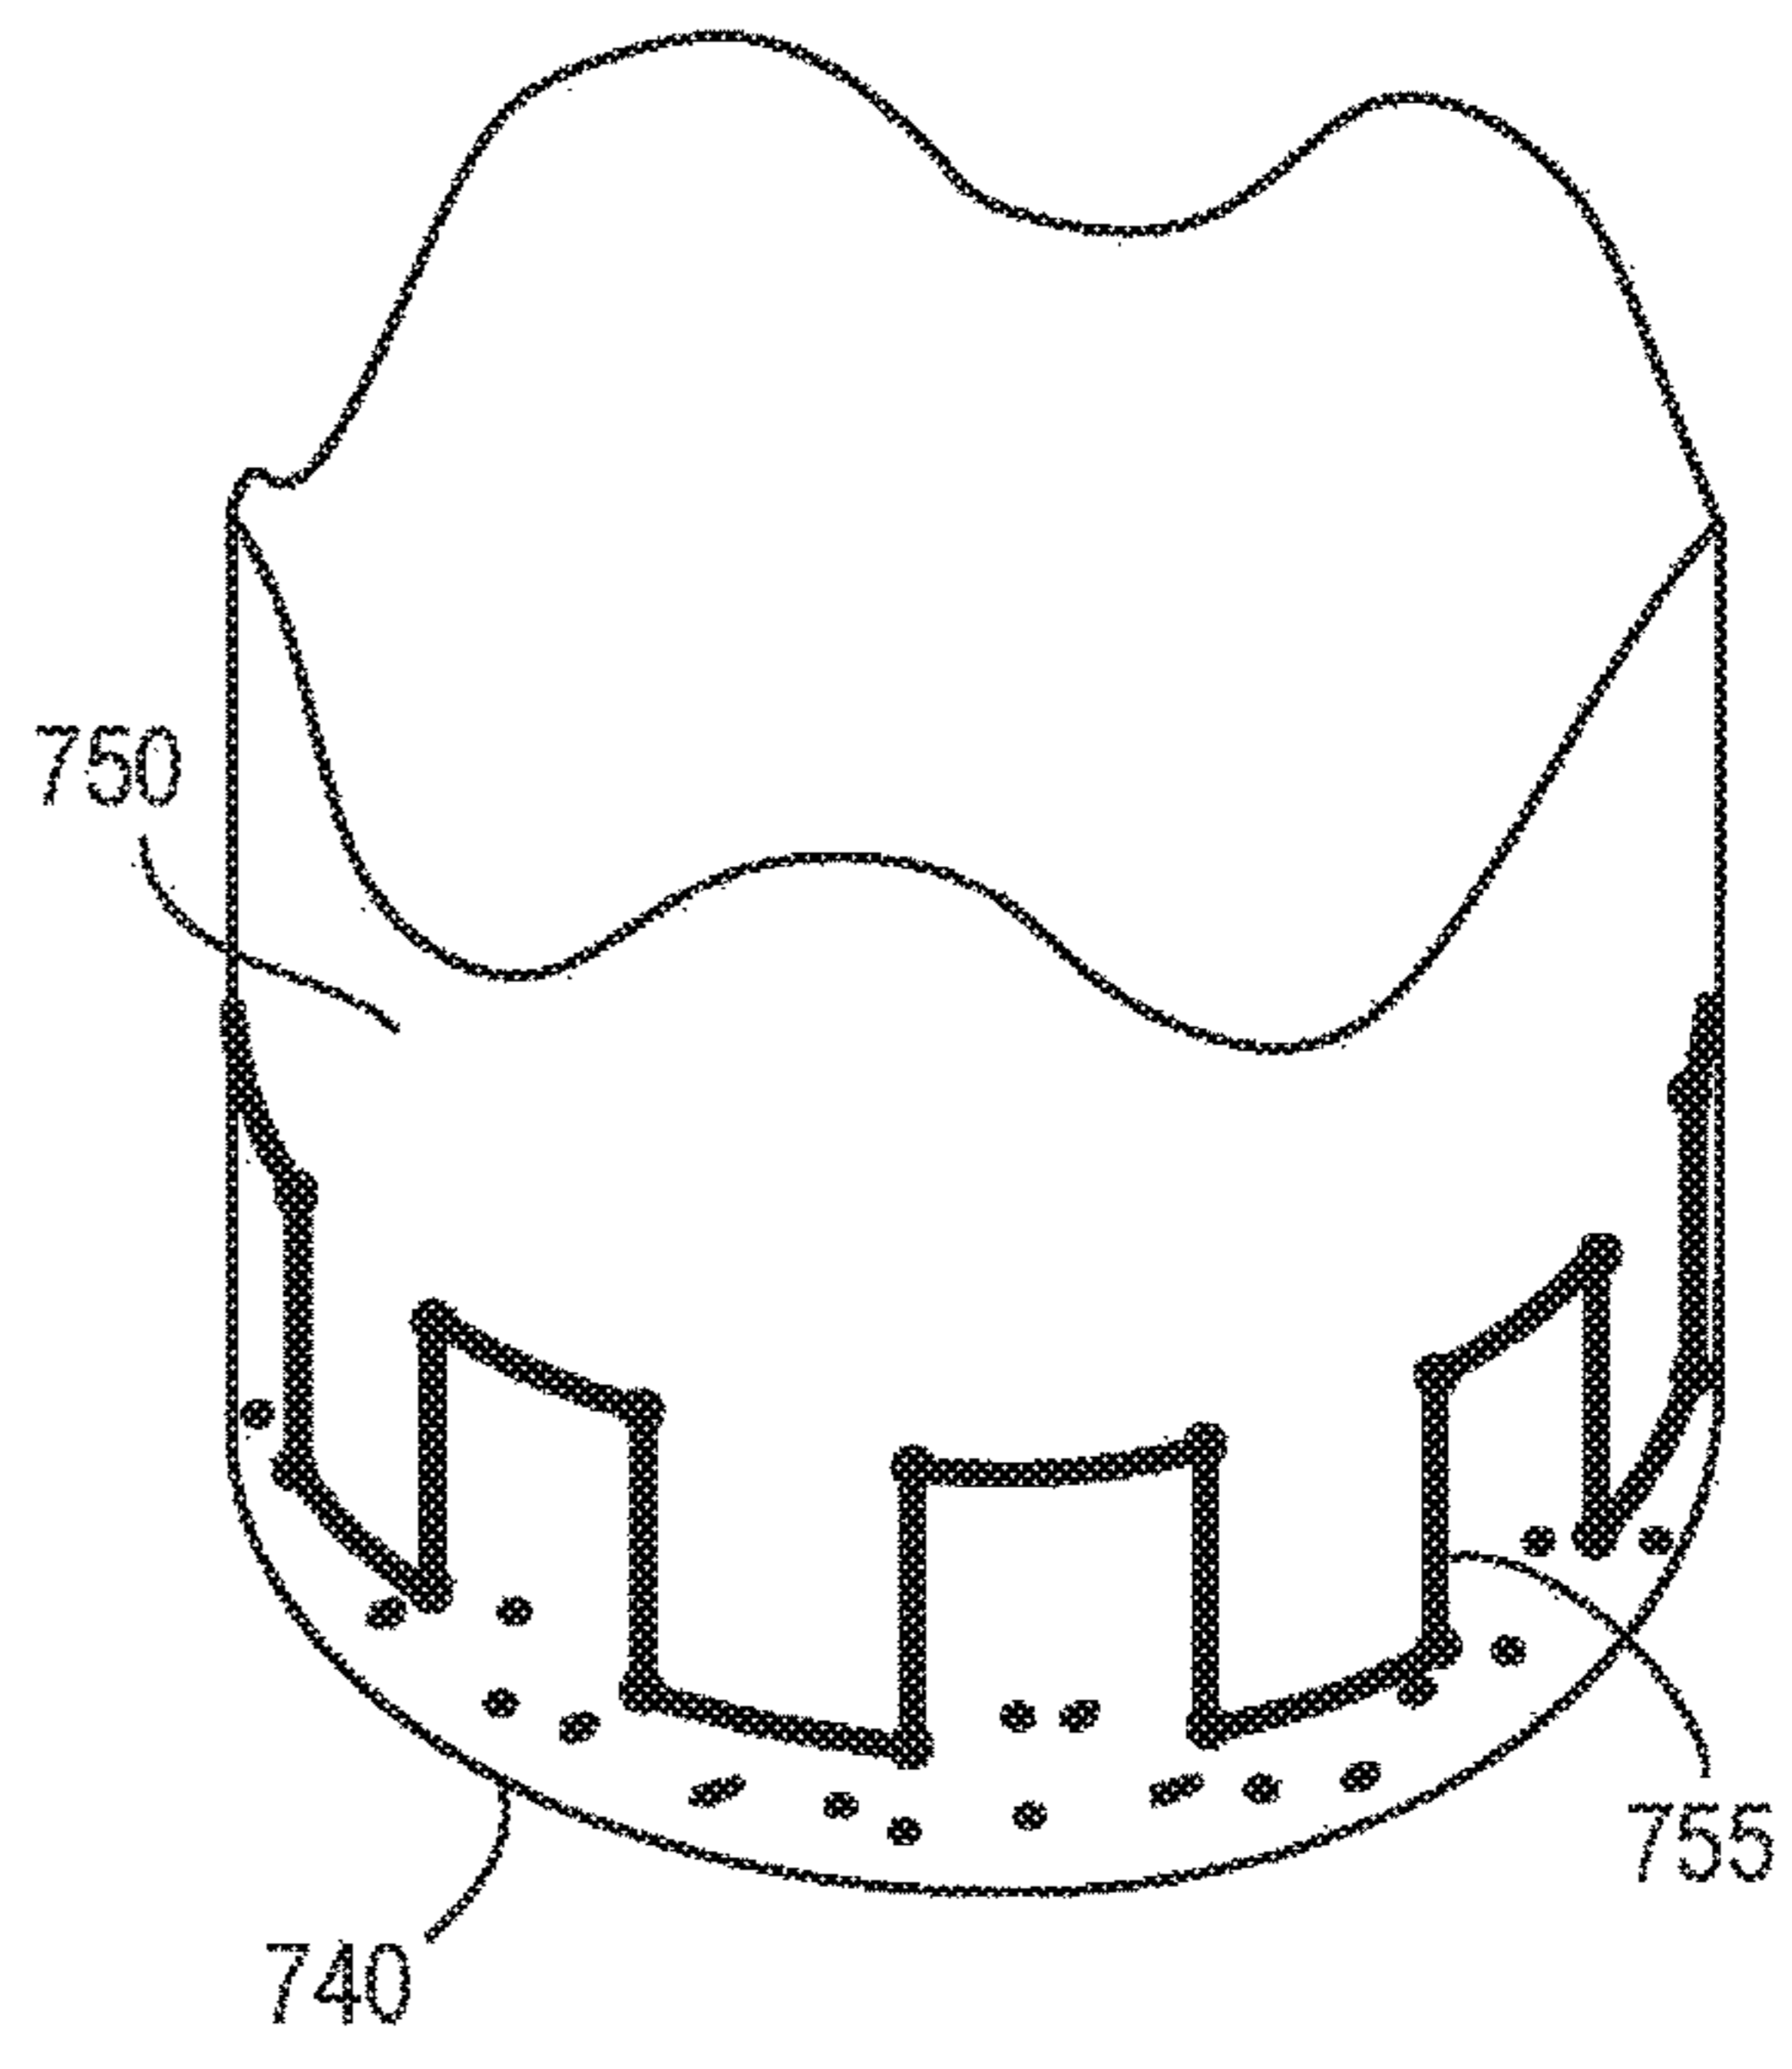


FIG. 7C

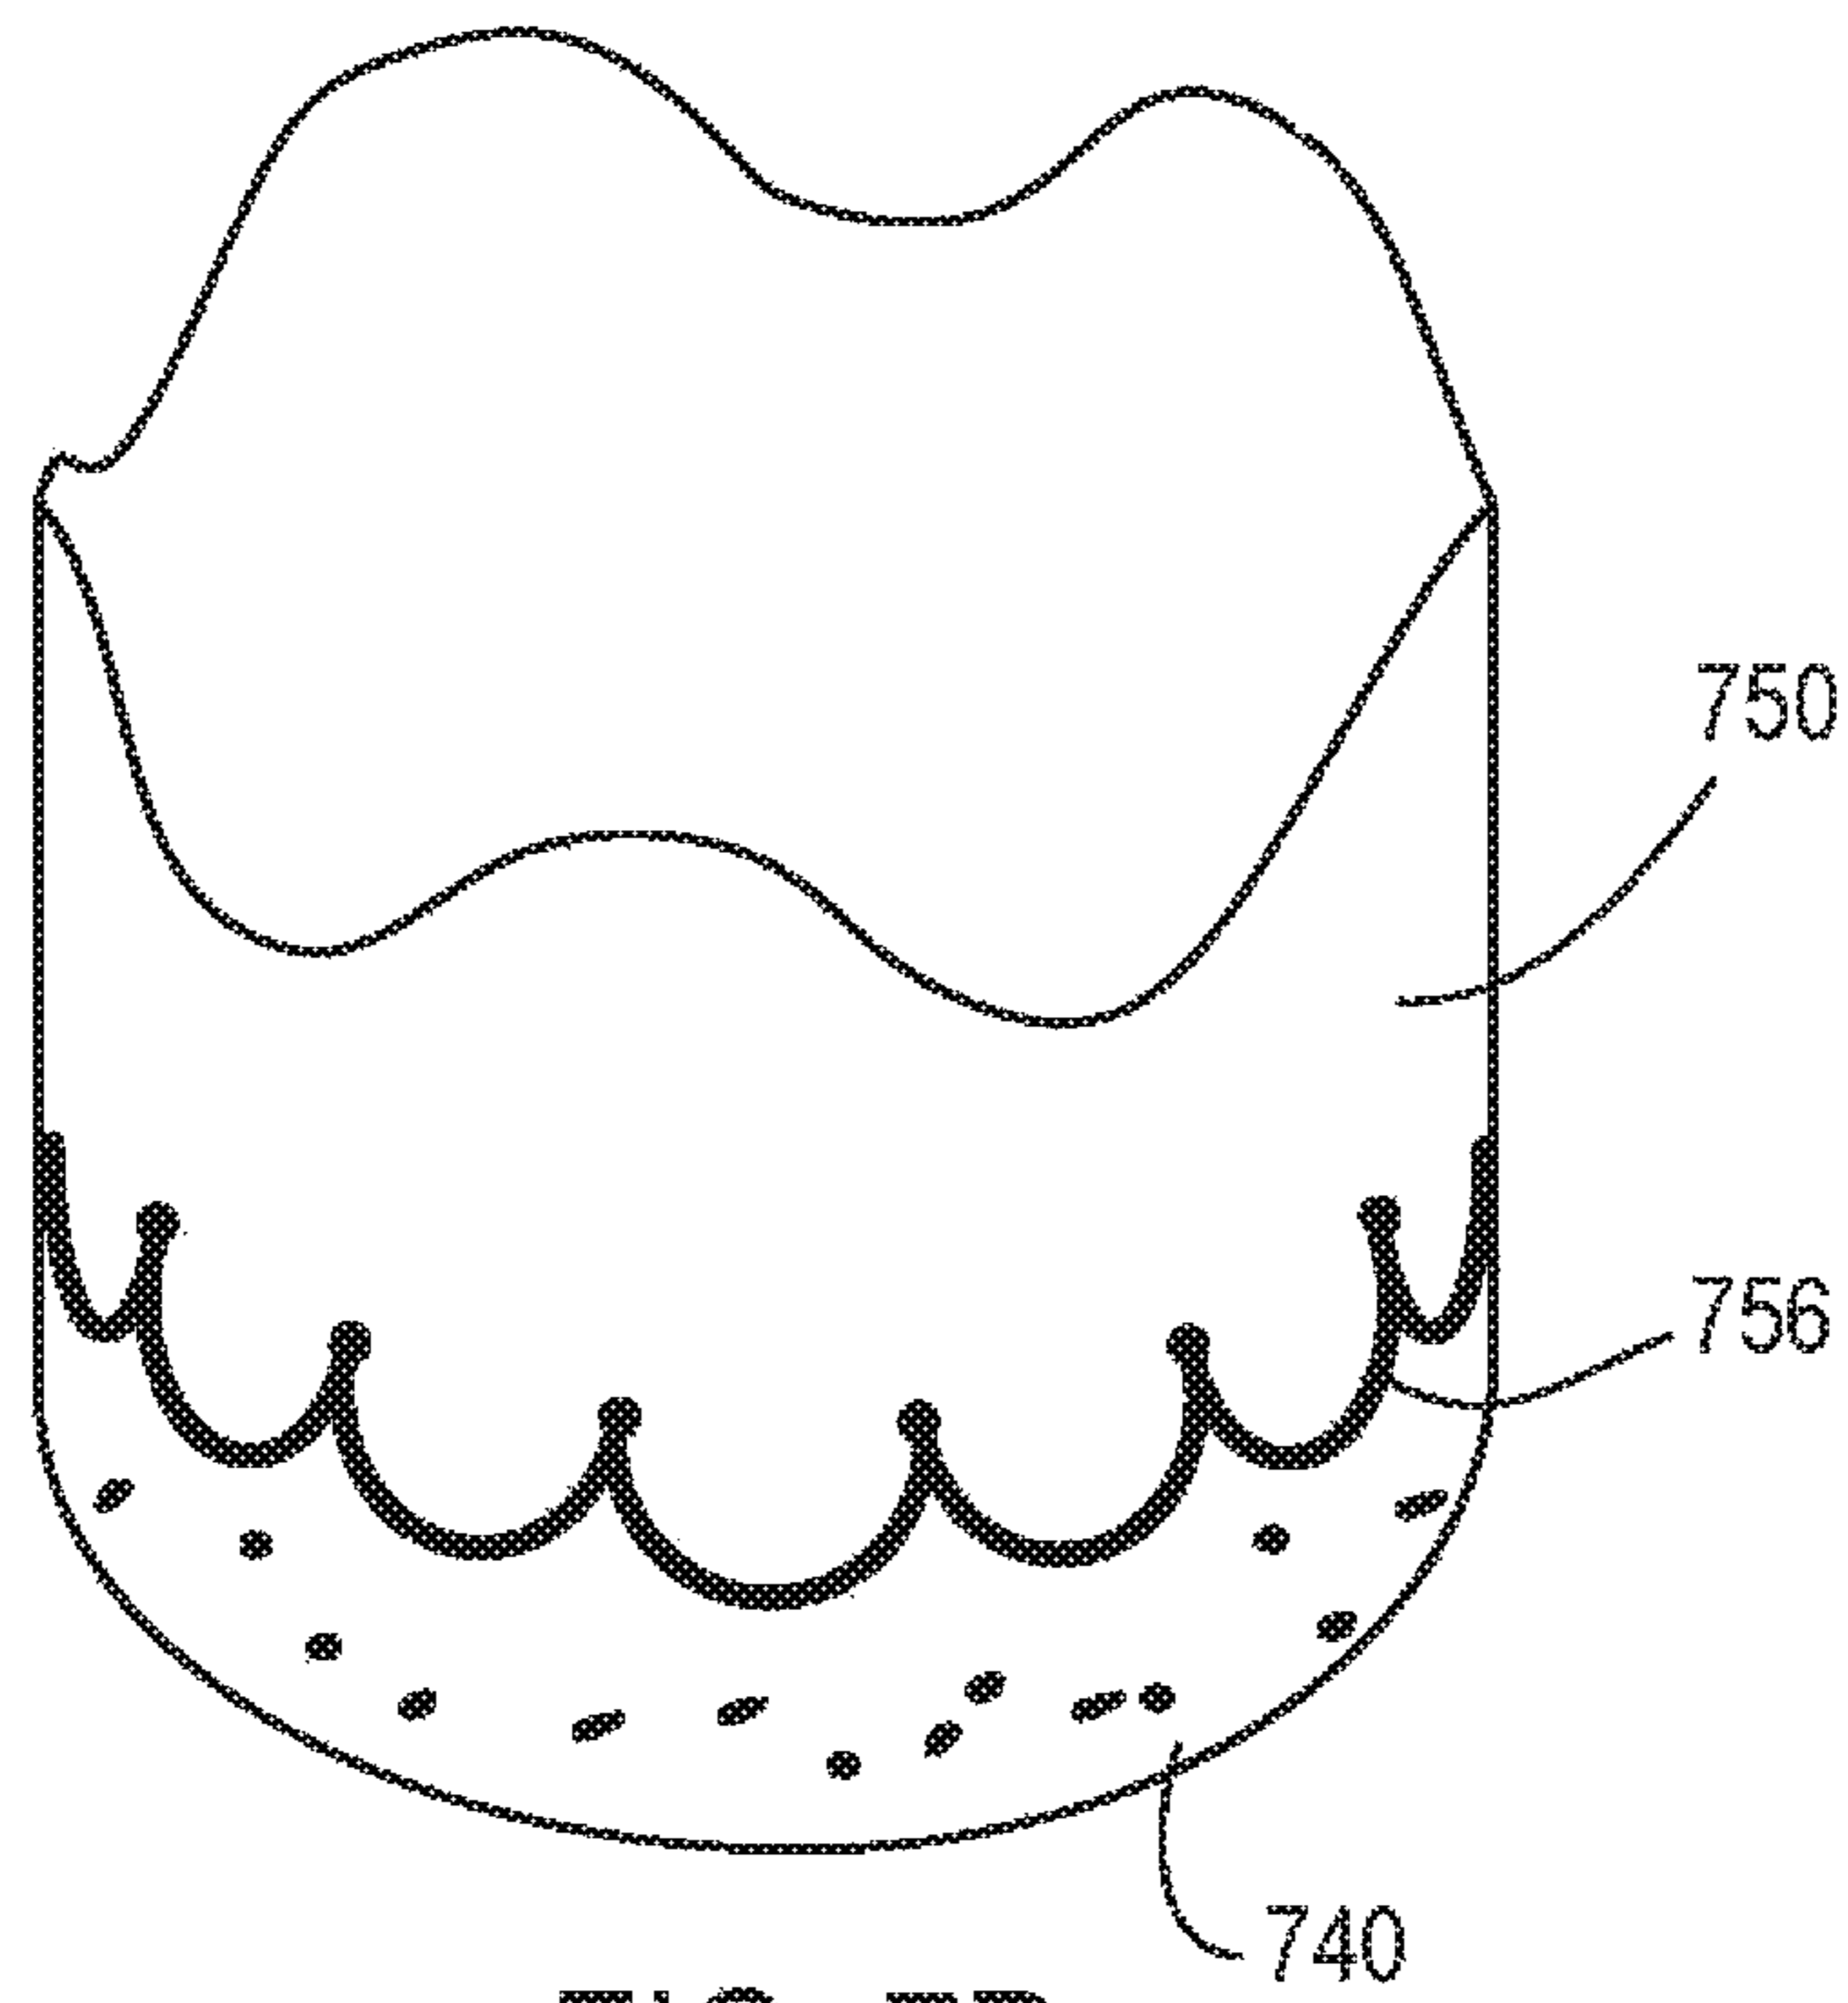


FIG. 7D

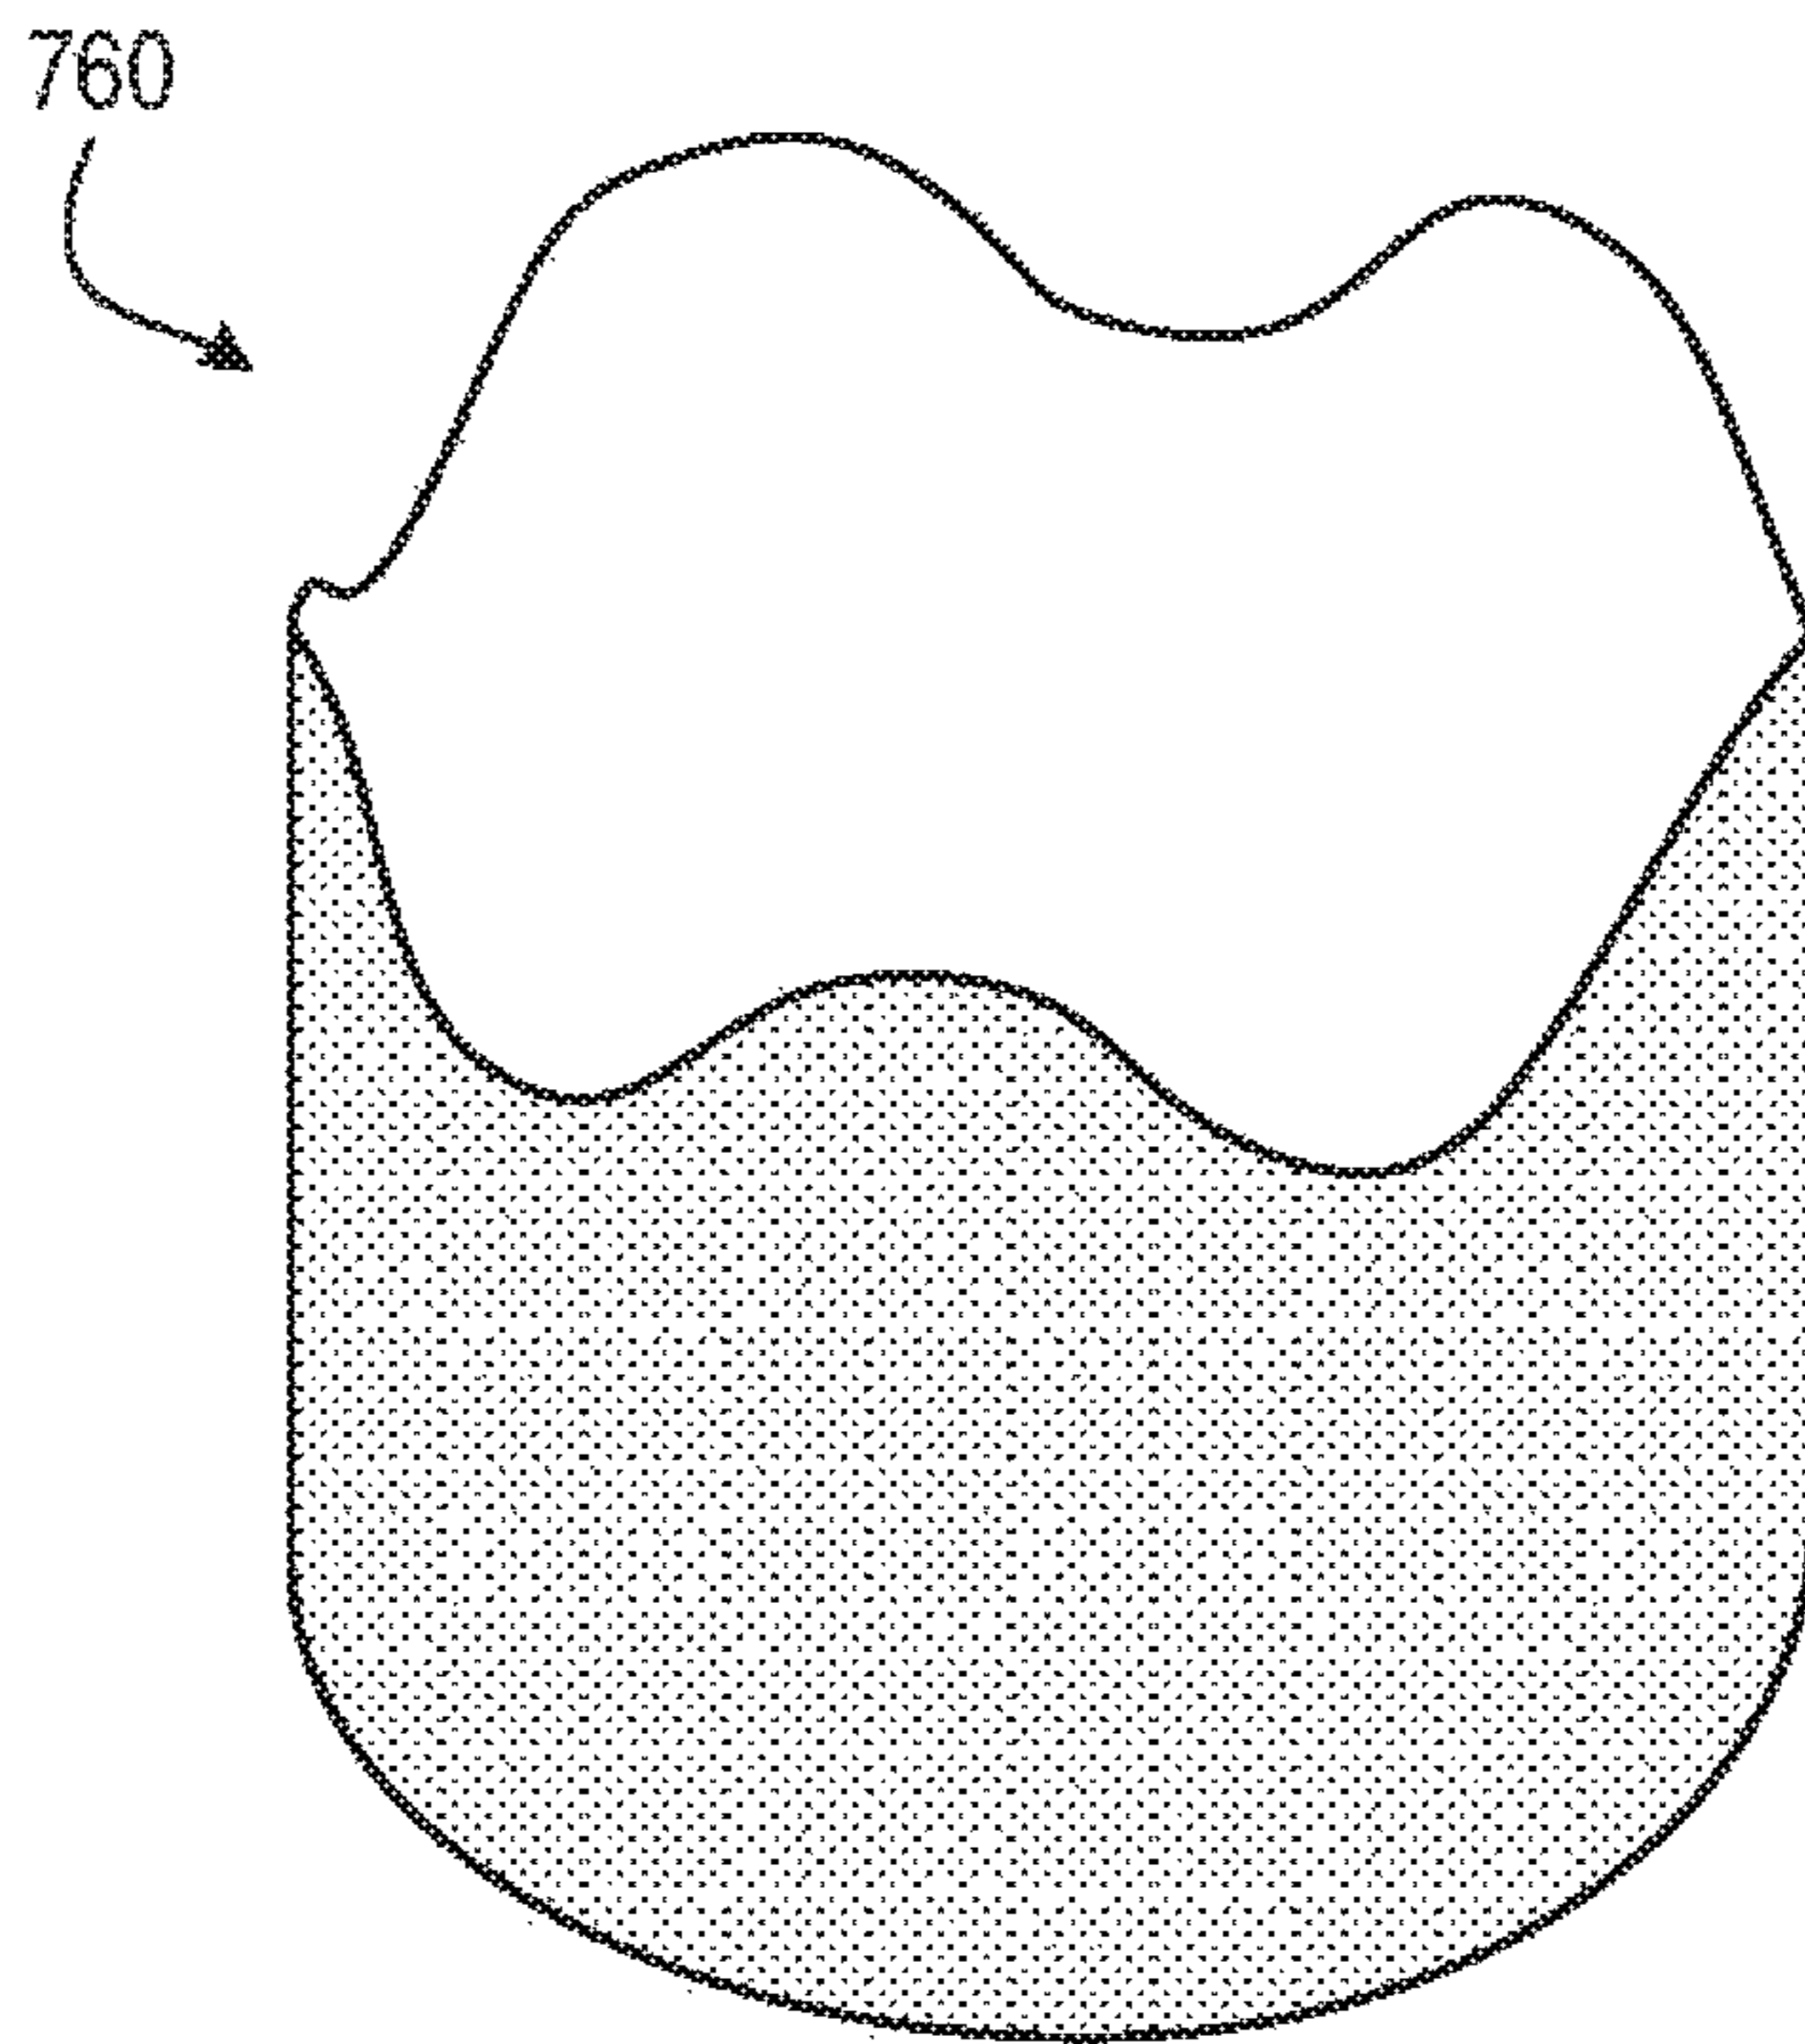


FIG. 7E

1

PROSTHETIC HEART VALVE HAVING TUBULAR SEAL

RELATED APPLICATIONS

This application claims the benefit of U.S. Provisional Application No. 62/111,472, file Feb. 3, 2015.

FIELD

This document provides prosthetic heart valves having a tubular seal.

BACKGROUND

The human heart contains four valves: a tricuspid valve, a pulmonic valve, a mitral valve and an aortic valve. The main purpose of the valves is to maintain unimpeded forward flow through the heart and into the major blood vessels connected to the heart, for example, the pulmonary artery and the aorta. As a result of a number of disease processes, both acquired and congenital, any one of the four heart valves may malfunction and result in either stenosis (impeded forward flow) and/or backward flow (regurgitation). Either process burdens the heart and may lead to serious problems, for example, heart failure. Various procedures for fixing or replacing defective heart valves are known in the art. In some cases, artificial heart valves can be implanted in the heart of a patient to replace a diseased or damaged heart valve with a prosthetic equivalent.

Prosthetic heart valves can have a variety of designs. Two major types of prosthetic heart valves include mechanical heart valves and bioprosthetic heart valves. Mechanical heart valves can be made of synthetic materials, such as plastics or metals, while bioprosthetic heart valves can be made of biologic tissue mounted on a fabric covered plastic or metal frame. Bioprosthetic heart valves can include animal tissue, such as porcine or bovine tissue, that has been chemically treated to make the valve suitable for implantation in a human. Bioprosthetic valves do not generally require a patient to undergo anticoagulant therapy, which is typically required when using mechanical valves. As such, there is a need to further improve the design of bioprosthetic valves to retain its functionality during the life of the patient and minimize stenosis and regurgitation.

SUMMARY

Prosthetic heart valves provided herein can have a structure adapted to retain functionality during the life of the patient and minimize stenosis and/or regurgitation by having an improved connection between different parts of a prosthetic heart valve.

In Example 1, a prosthetic heart valve includes an expandable member comprising one or more braided wires, the one or more braided wires comprising a first set of wire segments extended helically in a first direction and a second set of wire segments extended helically in a second direction such that each wire segment of the first set intersects a plurality of wire segments from the second set at a plurality of intersection points, wherein the one or more braided wires have crowns where the wire segments of the first set connect to wire segments of the second set. The prosthetic heart valve can additionally include a plurality of leaflets being secured within the expandable member and a tubular seal comprising an elastomeric material, the tubular seal having an inflow edge being secured to bottom inflow edges of the plurality

2

of leaflets and to the expandable member by a plurality of sutures, characterized by the sutures comprising cross stitches formed around both a wire segment of the first set and a wire segment of the second set at one of the intersection points.

In Example 2, the prosthetic heart valve of Example 1, wherein each cross stitch is an independently tied off stitch unconnected to other cross stitches.

In Example 3, the prosthetic heart valve of either Example 1 or Example 2, wherein each cross stitch is attached at an intersection point immediately adjacent a crown at an inflow side of the expandable member.

In Example 4, the prosthetic heart valve of any of Examples 1-3, wherein the plurality of leaflets are secured together along side edges thereof.

In Example 5, the prosthetic heart valve of Example 4, wherein the plurality of leaflets each comprise two sleeve portions, wherein the sleeve portions are secured to the expandable member by a plurality of anchor elements.

In Example 6, the prosthetic heart valve of any of Examples 1-5, wherein the tubular seal comprises a plurality of non-elastic fibers retained within a matrix of the elastomeric material, the non-elastic fibers being arranged to allow the tubular seal to stretch in an axial or a radial direction.

In Example 7, the prosthetic heart valve of Example 6, wherein the non-elastic fibers are part of a fabric.

In Example 8, the prosthetic heart valve of Example 7, wherein the fabric is a woven fabric.

In Example 9, the prosthetic heart valve of Example 8, wherein the woven fabric comprises fibers in a warp direction and fibers in a waft direction, wherein the fibers in both the warp direction and the waft direction are angled with respect to a central axis of the tubular seal.

In Example 10, the prosthetic heart valve of Example 9, wherein the fibers in both the warp direction and the waft direction are angled at an angle between 5 degrees and 70 degrees with respect to the central axis of the tubular seal.

In Example 11, the prosthetic heart valve of Examples 6-10, wherein the non-elastic fibers are uniformly dispersed throughout the elastomeric polymer matrix.

In Example 12, the prosthetic heart valve of Example 11, wherein the tubular seal has a substantially uniform thickness.

In Example 13, the prosthetic heart valve of any of Examples 1-10, wherein the tubular seal comprises an outflow end region and an inflow end region, the inflow end region being a portion of the tubular seal comprising a fabric within a matrix of the elastomeric matrix, wherein the fabric has a non-linear edge defining an interface between the inflow end region and the outflow end region.

In Example 14, the prosthetic heart valve of Example 13, wherein the non-linear edge of the fabric has a sinusoidal or scalloped shape.

In Example 15, the prosthetic heart valve of any of Example 1-14, wherein the plurality of leaflets are secured to the tubular seal by a continuous circumferential running stitch.

In Example 16, a prosthetic heart valve can include an expandable member comprising one or more braided wires, the one or more braided wires comprising a first set of wire segments extended helically in a first direction and a second set of wire segments extended helically in a second direction such that each wire segment of the first set intersects a plurality of wire segments from the second set at a plurality of intersection points, wherein the one or more braided wires have crowns where the wire segments of the first set connect to wire segments of the second set. The prosthetic heart

valve can additionally include a plurality of leaflets being secured within the expandable member and a tubular seal comprising an elastomeric material, the tubular seal having an inflow edge being secured to bottom inflow edges of the plurality of leaflets and to the expandable member by a plurality of sutures, characterized by the sutures comprising cross stitches formed around both a wire segment of the first set and a wire segment of the second set at one of the intersection points.

In Example 17, the prosthetic heart valve of Example 16, wherein each cross stitch is an independently tied off stitch unconnected to other cross stitches.

In Example 18, the prosthetic heart valve of Example 16, wherein each cross stitch is attached at an intersection point immediately adjacent a crown at an inflow side of the expandable member.

In Example 19, the prosthetic heart valve of Example 16, wherein the plurality of leaflets are secured together along side edges thereof.

In Example 20, the prosthetic heart valve of Example 19, wherein the plurality of leaflets each comprise two sleeve portions, wherein the sleeve portions are secured to the expandable member by a plurality of anchor elements.

In Example 21, the prosthetic heart valve of Example 16, wherein the tubular seal comprises a plurality of non-elastic fibers retained within a matrix of the elastomeric material, the non-elastic fibers being arranged to allow the tubular seal to stretch in an axial or a radial direction.

In Example 22, the prosthetic heart valve of Example 21, wherein the non-elastic fibers are part of a fabric.

In Example 23, the prosthetic heart valve of Example 22, wherein the fabric has a thickness ranging from about 40 to about 80 microns.

In Example 24, the prosthetic heart valve of Example 22, wherein the fabric is a woven fabric.

In Example 25, the prosthetic heart valve of Example 24, wherein the woven fabric comprises fibers in a warp direction and fibers in a waft direction, wherein the fibers in both the warp direction and the waft direction are angled with respect to a central axis of the tubular seal.

In Example 26, the prosthetic heart valve of Example 25, wherein the fibers in both the warp direction and the waft direction are angled at an angle between 5 degrees and 70 degrees with respect to the central axis of the tubular seal.

In Example 27, the prosthetic heart valve of Example 22, wherein the fibers are made of polyester.

In Example 28, the prosthetic heart valve of Example 21, wherein the non-elastic fibers are uniformly dispersed throughout the matrix.

In Example 29, the prosthetic heart valve of Example 16, wherein the tubular seal has a substantially uniform thickness.

In Example 30, a prosthetic heart valve includes an expandable member comprising one or more braided wires, the one or more braided wires comprising a first set of wire segments and a second set of wire segments such that each wire segment of the first set intersects a plurality of wire segments from the second set at a plurality of intersection points. The prosthetic heart valve can also include a plurality of leaflets secured within the expandable member and a tubular seal including an elastomeric material. The tubular seal can have an inflow edge being secured to bottom inflow edges of the plurality of leaflets and to the expandable member by a plurality of sutures. The sutures can include cross stitches formed around both a wire segment of the first set and a wire segment of the second set at one of the intersection points, wherein the tubular seal comprises an

outflow end region and an inflow end region. The inflow end region can be a portion of the tubular seal including a fabric within a matrix of an elastomeric matrix, wherein the fabric has a non-linear edge defining an interface between the inflow end region and the outflow end region.

In Example 31, the prosthetic heart valve of Example 30, wherein the non-linear edge of the fabric has a sinusoidal or scalloped shape.

In Example 32, the prosthetic heart valve of Example 30, wherein the plurality of leaflets are secured to the tubular seal by a continuous circumferential running stitch.

In Example 33, the prosthetic heart valve of Example 30, wherein the first set of wire segments extends helically in a first direction and a second set of wire segments extends helically in a second direction.

In Example 34, the prosthetic heart valve of Example 33, wherein the one or more braided wires have crowns where the wire segments of the first set connect to wire segments of the second set.

In Example 35, a method of making a tubular seal of a prosthetic heart valve includes forming a tubular seal that includes a fabric within a matrix by dipping a mandrel with a first coating composition that has at least one elastomeric polymer. The method can also include drying the first coating composition. The method can also include positioning the fabric on the mandrel and applying a second coating composition on the mandrel. The second coating composition can be different than the first coating composition. The method can further include removing the tubular seal from the mandrel.

The details of one or more embodiments of the invention are set forth in the accompanying drawings and the description below. Other features, objects, and advantages of the invention will be apparent from the description and drawings, and from the claims.

DESCRIPTION OF DRAWINGS

FIGS. 1A-1H illustrate an exemplary prosthetic heart valve and an exemplary deployment device provided herein. FIG. 1A is a perspective view of the heart valve connected to the deployment device. FIG. 1B is a side view of the exemplary prosthetic heart valve. FIGS. 1C-1H illustrate how the exemplary heart valve provided herein can be delivered by the deployment device.

FIGS. 2A-2C illustrates an exemplary leaflet, which can be used in prosthetic heart valves provided herein. FIG. 2A illustrates a rounded notch in a leaflet where a leaflet can be secured to an adjacent leaflet. FIGS. 2B and 2C illustrate a portion of an exemplary leaflet for prosthetic heart valves. FIG. 2B depicts the rounded notch in an armpit of a leaflet. FIG. 2C depicts attachment elements in the armpit of the leaflet.

FIG. 3 illustrates another exemplary leaflet, which can be used in prosthetic heart valves provided herein. FIG. 3 depicts apertures in a body of the exemplary leaflet.

FIGS. 4A-4G illustrate how adjacent leaflets can be stitched together in prosthetic heart valves provided herein.

FIGS. 5A-5C illustrate a cross stitch provided herein for connecting a seal to a braided stent in an exemplary prosthetic heart valve provided herein. FIG. 5A shows a front view of a seal having apertures and stitch patterns used for securing the seal to the braided stent. FIG. 5B depicts a close up view of a cross stitch and a portion of a circumferential stitch used for securing the seal to the braided stent. FIG. 5C depicts a cross-sectional view showing the cross stitch and a portion of the circumferential stitch.

FIG. 6 depicts an apparatus that can be used to form a tubular seal provided herein.

FIGS. 7A-7E depict exemplary tubular seals having a fabric positioned within a matrix that can be used in a prosthetic heart valve provided herein.

Like reference symbols in the various drawings indicate like elements.

DETAILED DESCRIPTION

Prosthetic heart valves provided herein can include a braided stent expandable member secured to a tubular seal using a plurality of cross stitches at a plurality of intersection points of wires of the braided stent. Stitching at intersection points (e.g., intersection points immediately adjacent to inflow crowns) as opposed to at inflow crowns can increase the strength of the attachment while also allowing for improved load transfer to the braided stent. Each stitch, which is described in further detail below, can be formed by passing two stitches of suture in orthogonal directions over the wire intersections, passing through the fabric strip in four locations. Each cross stitch can be individual knotted. In some cases, the cross stitches do not pass through any of the leaflets. The cross stitch can be repeated at many intersections circumferentially around an inflow end of a prosthetic heart valve provided herein until the entire length of the tubular seal is securely attached.

FIGS. 1A and 1B illustrate an exemplary prosthetic heart valve 100 provided herein. FIGS. 1C-1H depict how prosthetic heart valve 100 is deployed. FIG. 1A is a perspective view of prosthetic heart valve 100 connected to a deployment device 190. FIG. 1B is a side view of prosthetic heart valve 100. As shown, prosthetic heart valve 100 includes an expandable member 110, three leaflets 200, three anchor elements 120 that secure sleeve portions 216 of leaflets 200 to expandable member 110, and a tubular seal 130 secured around a blood inflow end of prosthetic heart valve 100. Anchor elements 120 can include post leg compression elements 122 and clamping support structures 126 adapted to provide support along opposite sides of the sleeve portions 216. Expandable member 110 in FIGS. 1A-1D is a braided stent, which is adapted to transition between a restricted state having a smaller diameter and an expanded state having a larger diameter. Expandable member 110 can be self-expanding, mechanically expanded, or a combination thereof.

FIGS. 1C-1H depict how an exemplary heart valve delivery system can deliver the prosthetic heart valve provided herein. As shown in FIGS. 1C-1H, prosthetic heart valve 100 can be deployed using a heart valve delivery system 180. System 180 can include a sheath 182 for retaining the prosthetic heart valve 100 with the expandable member 110 in a restricted state. Within sheath 182, anchor elements 120 (FIGS. 1A and 1B) can be connected to pushing prongs 192 and a pull line 194 can be connected to a nose cap 196, or end cap, which is positioned at the end of the sheath 182. As shown in FIG. 1A, the pull line 194 can extend through expandable member 110 and through the valve opening between the leaflets 200. As shown by FIGS. 1D-1H, once a distal end of sheath 182 is delivered through the circulatory system to an appropriate location (e.g., within the heart), prosthetic heart valve 100 can be deployed. By advancing pushing prongs 192 and pull line 194 relative to sheath 182, prosthetic heart valve 100 can be pushed out of the sheath 182. In some cases, expandable member 110 can self-expand upon exiting sheath 182. In some cases, expandable member 110 can self-expand to a first intermediate diameter, and

system 180 can mechanically expand expandable member 110 to a larger deployment diameter. For example, anchor elements 120 can include a locking mechanism to clip a portion of expandable member when the expandable member 110 is expanded to a predetermined locking diameter. In some cases, system 180 can mechanically expand expandable member 110 to a predetermined locking diameter. In some cases, system 180 can compress expandable member 110 between pushing prongs 192 and nose cap 196 by moving pull line 194 relative to pushing prongs 192. The predetermined locking diameter can be adapted to set the diameter of the prosthetic heart valve 100 during implantation. After prosthetic heart valve 100 is set, system 180 can move pull line 194 and nose cap 196 relative to pushing prongs 192 to move the end cap through the opening between leaflets 200 in prosthetic heart valve 100. Pushing prongs 192 can then be retracted from anchor elements 120 and retracted into sheath 182. In some cases, pushing prongs 192 can include a shape member material adapted to help radially expand expandable member 110 as the expandable member 110 exits sheath 182. A control handle 188 can be used to control the relative movements of sheath 182, pushing prongs 192, and pull wire 194. Prosthetic heart valves provided herein can be adapted to mitigate damage that might otherwise occur to valves during delivery and implantation.

In some cases, one or more radiopaque markers can be secured to prosthetic heart valves provided herein. As shown in FIGS. 1A and 1B, expandable member 110 includes a radiopaque marker 112. Any suitable radiopaque material (such as platinum, palladium, gold, tantalum, or alloys thereof) can be used as the radiopaque material in radiopaque marker 112. One or more radiopaque markers can be used with an imaging system to help a physician ensure that a valve is set in an appropriate location. In some cases, prosthetic heart valves provided herein include at least three radiopaque markers.

As shown in FIG. 1A, prosthetic heart valve 100 can include a plurality of leaflets 200. In some cases, as shown, prosthetic heart valve 100 includes three leaflets 200. In some cases, prosthetic heart valves provided herein can have any suitable number of leaflets, such as two, three, four, five, or more leaflets. In some cases, leaflets 200 are secured to one another. In some cases, leaflets 200 can be secured to one another via a plurality of sutures. Leaflets 200 can be sutured along side edges of a body portion of each leaflet. In some cases, prosthetic heart valves provided herein can include a single line of sutures, which can be adapted to minimize leaks, minimize the width of a seam, and/or minimize the profile of a replacement heart valve during percutaneous insertion. In some cases, prosthetic heart valves provided herein can include multiple lines of sutures.

Expandable member 110 can have any suitable structure, arrangement, or material. In some cases, expandable member 110 can include a braided wire stent. For example, U.S. Publication Number 2005/0143809, titled, "Methods and Apparatus for Endovascularly Replacing a Heart Valve," and filed on Nov. 5, 2004, which is herein incorporated by reference for its disclosure of possible structures and materials for a braided wire stent, discloses a braided wire stent. In some cases, expandable member 110 includes a shape memory material (e.g., a nickel-titanium alloy or a cobalt-chromium alloy).

Referring to FIGS. 2A-2C, a leaflet 200 can include a body portion 214 and sleeve portions 216. In some cases, the body portion 214 has a bottom edge 222, a first side edge 226, a second side edge 228, and a free edge 224. Leaflet 200

further includes a front (i.e., the side that blood flows toward), a back (i.e., the side that blood flows away from), a first side adjacent to the first side edge **226**, and a second side adjacent to the second side edge **228**. In some cases, the front of the leaflet **200** has a different texture than the back. In some cases, for example, the back of the leaflet may be prone to calcium build due to its cusp-shaped surface, therefore it can be beneficial to have a textured surface on the back of the leaflet to mitigate valve calcification issues. In some cases, however, having the back with a non-textured surface can mitigate calcification issues. In some cases, the leaflet **200** is made from tissue obtained from an animal, e.g., a pig or a cow. In some cases, leaflet **200** is made from bovine pericardium. Leaflets **200** can also be made from a synthetic material. Leaflets **200** can be assembled into a heart valve by aligning the opposite side regions of at least two adjacent leaflets **200** and stitching the leaflets **200** together along stitch line **246**, as shown in FIG. **2C**.

As shown in FIGS. **2A-2C**, a prosthetic heart valve can include at least one leaflet **200** having a body portion **214** and two opposite sleeve portions **216**. The body portion **214** can be defined by two side edges **226**, **228** adjacent each sleeve portion **216**. The at least one leaflet **200** can define at least one notch **232**, **234** between at least one of the two side edges **226**, **228** and the adjacent sleeve portion **216**. In other words, each notch **232**, **234** can be located along the side edges **228**, **226** at a location that is adjacent to the sleeve portions **216**, at an armpit of the leaflet **200**, as depicted in FIGS. **2A** and **2B**. In some cases, leaflet **200** can define a notch **232**, **234** generally along the side edges **228**, **226**. In some cases, a notch **232**, **234** can be defined along the sleeve portion **216**. In some cases, multiple notches **232**, **234** can be located along the sleeve portion **216** or one of the side edges **228**, **226**, and/or at the armpit of the leaflet **200**.

As shown in FIGS. **2A** and **2B**, the body portion **214** of the leaflet can have a conical frustum shape defined by a bottom edge **222**, the first side edge **226**, the second side edge **228**, and a free edge **224**. In some cases, other suitable shapes for the body portion can be contemplated, for example, a generally square, rectangular, triangular or trapezoidal shaped body portion.

The sleeve portions, as shown in FIGS. **2A-2C**, can extend outwardly from the body portion of the leaflet **200**. Each sleeve portion may be angled away from free edge of the body portion. Sleeve portions can be generally rectangular-shaped extensions with lateral ends. In some cases, the sleeve portions can have rounded ends.

Still referring to FIGS. **2A-2C**, notches **232**, **234** can be generally U-shaped. Other suitable notch shapes can include, but are not limited to, a V-shaped, Z-shaped, rectangular-shaped and an oval-shaped notch. Notches can also have rounded edges to smooth the transition between a notch and the side edges **228**, **226** of the leaflet **200**. Notches **232**, **234** can have a length dimension that can range from about 0.02 inches to about 0.20 inches (or from about 0.5 millimeters (mm) to about 4 mm).

Referring to FIG. **2C**, notches **232**, **234** can be shaped and sized to accommodate attachment of post leg compression elements **122**. Post leg compression elements **122** can be a part of anchor elements **120** (shown in FIGS. **1A** and **1B**) that compress and restrain sleeve portions **216** along the same line as the stitch line **246**. A suture **258** can be used to apply an appropriate and consistent compressive force between the post leg compression elements **122** in order to prevent leakage through sleeve portions **216** of the leaflets **200**. Sutures that pierce the body portion **214** at or near the armpit of the leaflet, however, can pull, stretch and abrade

the surrounding adjacent tissue, creating stress concentrations at or near the armpit of the leaflet. Stress concentrators can result in tears forming in the leaflet material. Using notches **232** and **234** and post leg compression elements **122**, however, can minimize potential heart valve tearing caused by sutures at or near the armpit location. Notches **232**, **234** can be positioned proximate to the post leg compression elements near the armpit of the leaflet, e.g., between at least one of the two side edges **226**, **228** and the adjacent sleeve portion **216**, to create enlarged openings that suture **258** can pass therethrough without pulling or stretching the adjacent tissue. Accordingly, a notched leaflet **200** can improve valve opening capabilities and the reliability of prosthetic heart valves provided herein.

FIG. **3** illustrates another exemplary leaflet, which can be used in prosthetic heart valves provided herein. As shown in FIG. **3**, leaflet **300** can include a body portion **314** and at least two opposite sleeve portions **316**. The body portion **314** can be defined by at least two side edges **326**, **328** adjacent each sleeve portion **316**. Leaflet **300** can define two apertures **332** and **334**. Each aperture **332**, **334** can be positioned adjacent the side edges **326**, **328** and an adjacent sleeve portion **316**. Each aperture **332**, **334** can be adapted to secure one leaflet to an adjacent leaflet.

In some cases, the body portion **314** has a bottom edge **322**, a first side edge **326**, a second side edge **328**, and a free edge **324**. Leaflet **300** further includes a front, a back, a first side adjacent to the first side edge **326**, and a second side adjacent to the second side edge **328**. In some cases, the front of the leaflet **300** has a different texture than the back. In some cases, this occurs where the leaflet **300** is made from pig, cow, or other natural animal tissue. In some cases, leaflet **300** is made from bovine pericardium. Leaflets **300** can also be made from a synthetic material. Leaflets **300** can be assembled into a heart valve by aligning the opposite side regions of at least two adjacent leaflets **300** and stitching the leaflets **300** together along stitch line **246**, as shown in FIG. **2C**.

As shown in FIG. **3**, leaflet **300** defines apertures **332** and **334** adjacent the side edges **328**, **326** and adjacent the sleeve portions **316**. Apertures **332** and **334** can be generally circular in shape. Other suitable aperture shapes can include, for example, a rectangular, an oval, a triangular, or a diamond shape. In some cases, apertures **332**, **334** can have a length dimension or a diameter from about 0.02 inches to about 0.20 inches (or from about 0.5 mm to about 4 mm). In some cases, one or more apertures **332**, **334** can be located in the side edges **328**, **326** and/or the sleeve portions **316** of the leaflet **300**. In some cases, multiple apertures can be located in a region that is adjacent to the side edges **328**, **326** and the sleeve portions **316**.

Apertures **332**, **334** in the leaflets **300** can allow one leaflet to be secured to an adjacent leaflet. Similar to the notches discussed above, apertures **332** and **334** can be shaped and sized to accommodate attachment of post leg compression elements **122**. Referring back to FIGS. **1A** and **1B**, post leg compression elements **122** can be a part of anchor elements **120** that compress and restrain sleeve portions **216** along the same line as the stitch line **246**. A suture **258** can be used to apply an appropriate and consistent compressive force between the post leg compression elements **122** in order to prevent leakage through sleeve portions **216** of the leaflets **200**. As already discussed herein, sutures that pierce the body portion **214** at or near the armpit of the leaflet can create stress concentrations at or near the armpit of the leaflet that may result in tearing. Apertures **332** and **334** and post leg compression elements **122**, however,

can minimize this potential tearing caused by sutures near the armpit location. Apertures **332**, **334** can be positioned proximate to the post leg compression elements near the armpit location to create enlarged openings that suture **258** can pass therethrough without pulling or stretching the adjacent tissue. Accordingly, leaflets **300** used in prosthetic heart valves provided herein can improve the reliability of prosthetic heart valves provided herein.

FIGS. **4A-4G** depict how leaflets **200** can be connected (or jointed) with an improved stitch discussed herein. As shown, stitch **446** can be a single continuous line stitch traveling along a stitch line in a forward direction and back in a reverse direction. In some cases, stitch **446** can run along a leaflet from a bottom edge to a side edge of the leaflet (e.g., bottom edge **222** to side edge **226** of leaflet **200** in FIG. **2A-2B**). In some cases, stitch **446** can run from a side edge to a notch of a leaflet (e.g., side edge **226** to notch **234** of leaflet **200** in FIG. **2A-2B**).

As shown in FIGS. **4D-4G**, stitch **446** can include a plurality of perpendicular loop segments **434** extending through an aperture in the two leaflets, around outer side edges of the two attached leaflets, and back through the aperture. Stitch **446** can include a plurality of parallel segments **436** extending between adjacent apertures along the stitch line. Stitch **446** can include two perpendicular loop segments **434** extending through apertures formed in the stitch line. In some cases, a first perpendicular loop segment **434** for a first aperture in the stitch line is formed when the stitch is formed in the forward direction and a second perpendicular loop segment **434** for the first aperture is formed in the reverse direction. In some cases, parallel segments **436** made in a forward direction alternate between opposite sides of the two leaflets between each aperture in the stitch line. In some cases, parallel segments **436** made in a reverse direction are formed on an opposite side of the two leaflets from parallel segments **436** made in a forward direction. In some cases, opposite parallel segments **436** made in the forward and reverse directions can provide a continuous compressive force along the entire length of the stitch line. Perpendicular loop segments **434** can provide compressive force to reinforce a seal formed between the two leaflets along the stitch line.

Stitch **446** can include any appropriate number of perpendicular loop segments formed through any appropriate number of apertures. As shown, stitch **446** includes six perpendicular loop segments formed through six apertures (two perpendicular loop segments per aperture). In some cases, stitch **446** can include up to twelve perpendicular loop segments formed through six or more apertures. In some cases, a stitch connecting side edge segments of leaflets can be formed using between 3 and 20 apertures and include between 3 and 40 perpendicular loop segments. In some cases, apertures can be positioned from about 0.008 inches to about 0.4 inches apart (about 0.2 mm to about 10 mm apart). In some cases, apertures can be positioned from about 0.008 inches to about 0.4 inches (about 0.2 mm to about 10 mm) away from the side edges of the leaflets.

Stitch **446** can be formed in a process depicted in FIGS. **4A-4G**. As shown in FIG. **4A**, a thread needle **410** can be passed through aligned leaflet side edges **226a** and **226b** to create a first aperture at a location near bottom edges **222**, e.g., a location approximately 1 mm from the bottom edges **222**. The leaflet side edges **226a** and **226b** can be retained in a desired configuration by clamping the leaflets between clamp sides **422** and **424**. Needle **410** pulls a leading end **431** of a thread **432** through the first aperture. As shown in FIG. **4B**, needle **410** can then form a second aperture adjacent to

the first aperture along the stitch line (towards the leaflet sleeve portion) about 0.5 mm away from the first aperture to pull leading end **431** of thread **432** through the second aperture to form a first parallel segment. As shown in FIG. **4C**, a perpendicular loop segment **434** can be made by guiding needle **410** around the leaflet side edges and re-enter the second aperture from a backside. Thread **432** can be pulled through the second aperture until it sits firmly against the leaflet material (e.g., leaflet pericardium tissue). FIG. **4D** shows a second parallel segment, which can be made by pushing needle **410** through leaflet tissue along the stitch line to form a third aperture approximately 1 mm from the second aperture (towards the sleeve segments of the leaflet). As shown in FIG. **4E**, a second perpendicular loop segment **434** can be formed by again having needle **410** loop around the leaflet side edges and reenter the third aperture through the backside. This is repeated up to notch **234** to form a total of six parallel segments **436** and six perpendicular loop segments **434** in a forward direction, as shown in FIG. **4F**. The stitch pattern can then be repeated in a reverse direction towards the bottom edges **222** of the leaflets through the previously formed apertures. Accordingly, each aperture can include two perpendicular loop segments **434** and parallel segments on the opposite sides can be formed from the parallel segments that were created in the forward direction, as shown in FIG. **4G**. The method and stitches depicted in FIGS. **4A-4G** can be applicable to leaflets **200**, **300** discussed herein.

Stitch **446** and other stitches provided herein can improve the reliability of a seal formed along a stitch line, create fewer apertures through the leaflets, and simplify the stitching operation. Having fewer apertures can help minimize the occurrence of blood leakage through the apertures. The single continuous line of stitch **446** using a single row of apertures can minimize a width of a side edge portion needed to form a continuous seal along the side edges of the leaflets, thus providing a reduced restricted profile for prosthetic heart valves provided herein. For example, U.S. Pat. No. 8,778,020 describes a variety of ways that leaflets can be sutured together using combinations of whip stitches and running stitches, but these stitches require additional apertures and multiple lines. Perpendicular loop segments **434** can stitch a plurality of leaflets together, similar to the whip stitches discussed in U.S. Pat. No. 8,778,020. Parallel segments **436** can secure valve leaflets to one another, similar to the running stitches discussed in U.S. Pat. No. 8,778,020. Although stitch **446** can provide an improved attachment between side edges of leaflets in prosthetic heart valves provided herein, some embodiments of prosthetic heart valves provided herein can use other stitch patterns, such as those described in U.S. Pat. No. 8,778,020, which is hereby incorporated by reference.

Important characteristics of the thread can include, but are not limited to, tensile strength, abrasion resistance and creep rupture resistance characteristics that allow the device to be delivered and implanted into a human anatomy. The thread used for suturing together portions of the heart valve, e.g., sides edges of the leaflets, can be composed of biocompatible materials that include, but are not limited to, polyethylenes such as ultra high molecular weight polyethylene (UHMWPE), polyesters (PET), and combinations thereof.

Referring back to FIGS. **1A** and **1B**, prosthetic heart valve **100** can include a tubular seal **130**. Tubular seal **130** can be secured to bottom edges **222** (FIG. **2A**) of the body portion **214** of at least one leaflet **200** by a circumferential running stitch **134** within prosthetic heart valve **100**. Tubular seal **130** can be secured to expandable tubular member **110** by

11

fasteners **136** and extended around the outside of expandable tubular member **110** to provide a seal that minimizes blood leakage around the leaflets **200** of an implanted prosthetic heart valve **100**. The structure and materials of tubular seal **130** are discussed below in reference to FIGS. **6** and **7A-7E**.

Referring to FIGS. **5A-5C**, an improved tubular seal stitching pattern can include a cross stitch **132** between tubular seal **130** and expandable member **110**. FIGS. **5A-5C** illustrate how the tubular seal **130** can be secured to the expandable member **110**, e.g., a braided stent, by a plurality of cross stitches connecting the tubular seal **130** to a pair of overlapping wire members of the braided stent. As shown in FIGS. **1A**, **1B** and **5A-5C**, expandable member **110** can be a braided stent including one or more wires having a first set of segments **114** extending helically in a first direction and a second set of segments **116** extending helically in a second direction such that the first set of segments **114** cross the second set of segments **116** at intersection points **118**. As shown, one or more wires can have inflow crowns **115** at an end of the braided stent where the wires transition from first segments **114** to second segments **116**. In some cases, cross stitches **132** secure tubular seal **130** at an intersection **118** to two crossing segments **114**, **116** of the braided stent. A separate circumferential running stitch **134** can be inserted into preformed apertures **133** to secure the adaptive seal to bottom edges **222** of leaflets **200** shown in FIGS. **2A** and **2C**. Cross-stitches around the intersections **118** can increase the strength of an attachment of tubular seal **130** to the expandable member **110** while also allowing for improved load transfer to the expandable member **110**. In some cases, the cross stitches secure tubular seal **130** at intersections **118** located immediately above (proximal) the inflow crowns **115**. Cross stitches **132** can be formed by passing two stitches **132a**, **132b** of a suture in orthogonal directions over the intersections **118** and through the tubular seal **130**. In some cases, preformed apertures **131** for cross stitch **132** can

12

intersection **118** immediately adjacent to inflow crowns **115** is sutured to tubular seal **130** via a cross stitch provided herein. The tubular seal stitching pattern provided herein can increase the strength of the attachment between the tubular seal **130** and the expandable member **110** while also allowing for improved load transfer to the expandable member **110** through the use of the plurality of cross stitches.

Tubular seal **130** can have any suitable structure. In some cases, tubular seal **130** can include an elastic material. In some cases, tubular seal **130** can include one or more layers of an elastomeric polymer. In some cases, tubular seal **130** can include a polycarbonate, polyurethane, silicone, polytetrafluoroethylene (PTFE), or a combination thereof. Other suitable materials include, but are not limited to, natural and synthetic rubbers, including cis-1,4-polyisoprene rubber, styrene/butadiene copolymers, polybutadiene rubber, styrene/isoprene/butadiene rubber, butyl rubber, halobutyl rubber; polyurethane elastomers, including elastomers based on both aromatic and aliphatic isocyanates; flexible polyolefins, including flexible polyethylene and polypropylene homopolymers and copolymers; styrenic thermoplastic elastomers; polyamide elastomers; polyamide-ether elastomers; ester-ether or ester-ester elastomers; flexible ionomers; thermoplastic vulcanizates; flexible poly(vinyl chloride) homopolymers and copolymers; flexible acrylic polymers; and blends and alloys of these, such as poly(vinyl chloride) alloys like poly(vinyl chloride)-polyurethane alloys. In some cases, tubular seal **130** can include an aliphatic polycarbonate-based thermoplastic urethane. In some cases, tubular seal **130** can include an elastomeric polymer having a hardness ranging from 3.07 MPa to 9.9 MPa, or a durometer ranging from 75 Shore A to 75 Shore D using ASTM standard D2240 in force on Jan. 1, 2014. In some cases, tubular seal **130** can include a polymeric material having the mechanical properties shown in Table I below. Notably, all of the listed ASTM standards refers to the standard in force on Jan. 1, 2014.

TABLE I

				ASTM Standard
Durometer Range Available	75 Shore A-75 Shore D			D2240
Specific Gravity	1.10-1.14			D792
Melt Flow	2-26 g/10 min(205° C./3.26 kg)			D1238
	MECHANICAL PROPERTY RANGES			
				ASTM Standard
Durometer	75A-B20	55D	75D	75D
Ultimate Tensile Strength (psi)	400-9000	5000-10000	3000-8000	D638
Tensile (psi)				
@50% elongation	350-650	1500-1800	3000-8000	D638
@100% elongation	550-850	1800-2200	3000-8000	D638
@200% elongation	600-1200	2800-4200		D638
@300% elongation	1200-2000	4200-10000		D630
Ultimate Elongation (%)	350-750	200-400	100-300	D638

be formed in the tubular seal **130**. In some cases, a portion of the tubular seal **130** that is sutured by cross stitch **132** includes an internal fabric, such as those discussed below. Each cross stitch **132** can be knotted independently. As shown in FIG. **5C**, cross stitches **132** each include a separate knot **137**. Additionally, cross stitches **132** can be arranged to not pass through leaflets **200**. Cross stitches **132** can be repeated at a plurality of intersections **118** (FIG. **5A**) circumferentially around an inflow end of a prosthetic heart valve provided herein such that an entire circumference of tubular seal **130** is securely attached. In some cases, each

In some cases, referring back to FIG. **1A**, tubular seal **130** can include attachment structures to improve the attachment of the tubular seal **130** to leaflets **200** and/or expandable member **110**.

In some cases, as shown in FIG. **7A**, a tubular seal **730** can include an inflow end section **740** and an outflow end section **750**. The inflow end section **740** can include a fabric embedded within elastomeric material and the outflow end section **750** can include a plurality of grommets **732**. The fabric of inflow end section **740** can be a woven material. In some cases, the fabric can have warp threads and/or weft

threads. The fabric is composed of fibers having an average thread diameter from about 0.00002 inches to about 0.002 inches (or from about 0.5 microns to about 50 microns), more preferably from about 0.0008 inches to about 0.002 inches (or from about 20 micron to about 40 microns). In some cases, more preferably, the fabric is composed of fibers having a thread diameter of about 0.0011 inches (about 27 microns).

In some cases, the fabric can include non-elastomeric fibers. Suitable non-elastomeric fiber materials include, but are not limited to, polyolefins, polyesters such as PES 38/31 manufactured by SaatiTech, and polyamides. More particularly, the polyolefins may be, for example, one or more of polyethylene, polypropylene, polybutene, ethylene copolymers, propylene copolymers, and butene copolymers. Because the fabric can include non-elastic fibers, inflow end section **740** and outflow end section **750** can have different overall elastic properties. In some cases, tubular seal **730** can be used as a tubular seal **130** of prosthetic heart valve **100**, as previously shown in FIG. 1A. In some cases, tubular seal **730** can be used in other prosthetic heart valves provided herein.

As shown in FIGS. 7A-7D, an interface **753** between the inflow end section **740** and the outflow end section **750** is non-linear due to a non-linear edge of fabric within the inflow end section **740**. As shown in FIG. 7A, the non-linear edge can be sinusoidal **753**. In some cases, as shown in FIGS. 7C-7D, the non-linear edge can be a zigzagged edge **754**, a stepped edge **755**, or a scalloped edge **756**.

In some cases, inflow end section **740** can be thicker than outflow end section because of the presence of a fabric within inflow end section **740**, **750**. In some cases, inflow end section **740** can have a thickness of about 0.0028 inches (about 70 microns) and the outflow end section **750** can have a thickness of about 0.0020 inches (about 50 microns). Other suitable thicknesses for the inflow end section include thicknesses ranging from about 0.0020 inches to about 0.0035 inches (about 50 microns to about 90 microns), or more preferably, from about 0.0025 inches to about 0.0031 inches (about 60 microns to about 80 microns). Suitable thicknesses for the outflow end section include thicknesses ranging from about 0.0011 inches to about 0.0028 inches (about 30 microns to about 70 microns), or more preferably, from about 0.0016 inches to about 0.0023 inches (about 40 microns to about 60 microns). In some cases, suitable thickness ratios of the inflow end section relative to the outflow end section can range from 1:1 to 1.2:1, from 1.2:1 to 1.4:1, from 1.4:1 to 1.5:1, and from 1.5:1 to 2:1. A non-linear edge can providing a non-linear interface between the inflow end section **740** and the outflow end section **750**. A prosthetic heart valve with the non-linear interface may have an increased overall diameter that tapers more gradually when compared to a prosthetic heart valve that has a linear interface. The non-linear edge of the fabric can also gradually transition the change in elastic properties between the outflow end section **750** and the inflow end section **740**, mitigating the formation of stress concentrators along the interface **753** that can cause tearing in the tubular member. Additionally, the shape of non-linear interface **753** can limit the propagation of tears.

In some cases, the fabric can be arranged in the inflow end section **740** to allow for the fabric within inflow end section **740** to stretch in axial and/or radial directions to allow the tubular seal to stretch along with an expandable member during implantation. When the fabric does not allow the tubular seal to adequately stretch, the seal can cause non-uniform crimping during manufacturing or damage the

expandable member during device deployment. In some cases, a woven fabric can be arranged to have the warp and the waft extend in directions oblique to the axis of the tubular seal. This can allow the fabric to flex in radial and/or axial directions relative to the axis of the tubular seal, but limit the fabric from stretching in a direction oblique to the axis. In some cases, both the warp and the waft can extend at an angle between 30 degrees and 60 degrees with the axis of the tubular seal. In some cases, both the warp and the waft can extend at an angle between 5 degrees and 70 degrees with the axis of the tubular seal. In some cases, the warp and waft can be arranged within the tubular member **730** to form an angle of about 45 degrees with the axis of the tubular seal. In some cases, the fabric can be a knit fabric arranged to allow for a predetermined amount of stretch in the axial and/or radial directions. Limiting the fabric within inflow end section **740** from stretching in a direction oblique to the axis can prevent the fabric from bunching and minimize non-uniform crimping during manufacturing.

Additional exemplary tubular seals including a fabric and grommets are described in U.S. Patent Application No. 2013/0090729, which is hereby incorporated by reference in its entirety. For example, U.S. Pat. No. 8,778,020 describes a seal that includes a multilayer, cylindrical seal body having projections alternating with recesses along the proximal edge of the seal body with proximal reinforcing grommets and a distal reinforcing band, which may be formed from a woven or nonwoven fabric and either incorporated within the interior of the multilayer seal body or adhered to the surface thereof.

In some cases, tubular seals described in U.S. Patent Application No. 2013/0090729 can be modified to include a fabric arrangement that allows a seal to stretch in axial and/or radial directions. In some cases, elastomeric materials provided herein can be incorporated into the tubular seals disclosed in U.S. Patent Application No. 2013/0090729. In some cases, the tubular seals described in U.S. Patent Application No. 2013/0090729 can be modified to include the non-linear interface **753** provided herein.

Referring back to FIG. 7A, tubular seal **730** can be created by producing one or more layers of elastomeric polymer, applying the fabric and grommets **732** to the one or more layers of elastomeric polymer, and overcoating the fabric and grommets **732** with one or more additional layers of elastomeric material. In some cases, different layers can have different elastomeric properties. In some cases, tubular seals (e.g., **130**, **730**, or **760**) can include a radially innermost layer including at least one elastomeric polymer, e.g., a polycarbonate and a polyurethane; a radially outermost layer including at least one elastomeric polymer, e.g., a polycarbonate and a polyurethane; and at least one inner layer disposed between the radially outermost layer and a radially innermost layer. In some cases, the modulus of elasticity of the innermost layer is less than the modulus of elasticity of the radially innermost outer layer and the modulus of elasticity of the radially outermost outer layer. In some cases, the elongation to break of the inner layer is greater than the elongation to break of the radially innermost outer layer and the elongation to break of the radially outermost outer layer. Although the radially innermost outer layer and the radially outermost outer layer have been depicted as including the same material, it will be appreciated that they may be compositionally the same or different.

The multilayer tubular seals provided herein (e.g., **130**, **730**, **760**) may be formed in a variety of ways. In some cases, multilayer tubular seals provided herein may be formed by successive applications of a polymer solution to an appro-

priately shaped mandrel, such as that illustrated in FIG. 6. Following a careful cleaning of the mandrel **600**, the mandrel may be mounted to an appropriate holding fixture in a spray booth. A first coating composition including a carrier and at least one polymer may be applied to the mandrel **600** and subsequently dried to form a first coated mandrel. In some cases, the first coating composition includes one or more elastomeric polymers, e.g., polycarbonate and/or a polyurethane, and a volatile carrier. The coating composition may be applied as a single layer or multiple layers to achieve the desired dried coating thickness. The grommets **732** (FIG. 7A) and the fabric may be positioned on the first coated mandrel by inserting locating pins **620** in apertures **610** in the tapered mandrel **600** which align with corresponding perforations **30** provided in the grommets **32**, **34**, **36** and the fabric **40**. In FIG. 6, only one pin **620** has been illustrated for clarity. In some instances, it may be desirable to secure the plurality of grommets **732** and the fabric to the mandrel or to an underlying coating layer by applying a drop of a first coating composition, or other adhesive composition, to each item to ensure that it remains properly positioned during subsequent processing. The fabric can be cut to a suitable shape having a non-linear edge using any suitable method. In some cases, the fabric can be die cut. In some cases, the fabric can be cut with a blade. In some cases, the fabric can be cut using a femtosecond laser. In some cases, a femtosecond laser cut fabric mitigate the chances of forming stress concentrators along the edge of the fabric.

A second coating composition including a carrier and at least one polymer may be applied to the first coated mandrel, the fabric, and the plurality of grommets. In some cases, the second coating composition includes one or more elastomeric polymers, e.g., polycarbonate and/or a polyurethane, and a volatile carrier. The carrier of the second coating composition may be removed, thereby forming a second coated mandrel. The second coating composition may be applied as a single layer or as multiple layers to achieve the desired dried coating thickness. In some cases, the second coating composition may be different from the first coating composition. In some cases, the second coating composition may be composed of the same material as the first coating composition.

In some cases, a third coating composition including a carrier and at least one polymer may be applied to the second coated mandrel. In some cases, the third coating composition includes one or more elastomeric polymers, e.g., polycarbonate and/or a polyurethane, and a volatile carrier. The carrier of the third coating composition may be removed thereby forming a tubular seal precursor. The third coating composition may be applied as a single layer or as multiple layers to achieve the desired dried coating thickness. In some cases, the third coating composition may be different from the first coating composition. In some cases, the third coating composition may be the same as the first coating composition. In some cases, the third coating composition may be different from the second coating composition. In some cases, the third coating composition may be the same as the second coating composition. Following removal of the carrier from the third coating composition, the tubular seal precursor may be inspected to ensure that it is fully formed and meets dimensional specifications, such as a thickness specification. In some cases, a suitable thickness for the tubular seal precursor can range from about 0.001 inches to about 0.0030 inches (about 30 microns to about 75 microns) or from about 0.002 inches to about 0.0047 inches (about 50 microns to about 120 microns). Other suitable thicknesses for the tubular seal precursor include a range

from about 0.0008 inches to about 0.002 inches (about 20 microns to about 40 microns), about 0.001 inches to about 0.002 inches (about 30 microns to about 50 microns), about 0.002 inches to about 0.0029 inches (about 50 microns to about 75 microns), about 0.002 inches to about 0.004 inches (about 50 microns to about 100 microns), about 0.004 inches to about 0.0047 inches (about 100 microns to about 120 microns), about 0.004 inches to about 0.0059 inches (about 100 microns to about 150 microns), about 0.0059 inches to about 0.0079 inches (about 150 microns to about 200 microns), as well as any thickness value within any of the listed ranges.

In some cases, the tubular seal precursor may be inspected to ensure that it meets certain functional specifications, e.g., tensile and frictional specifications. The tubular seal precursor may then be trimmed by laser cutting, or blade cutting, to conform to dimensional specifications and removed from the tapered seal-forming mandrel as a formed tubular seal. In some cases, at least some preformed apertures for suturing tubular seal to expandable member **110** and/or leaflets **200** can be performed by laser cutting. In some cases, at least some of the grommets may be formed by a laser cutting operation performed on a tubular seal precursor. In some cases, grommets **732** of FIG. 7A may be added to the multilayer, generally cylindrical seal, in a step not illustrated, as a proximal band. Subsequent laser cutting of the tubular seal precursor would then simultaneously form grommets **732** by removing the portions of the proximal band located between the projections.

In some cases, coating compositions may be selected to provide a relatively stiff dried polymer such as a dried polymer having a Shore D hardness of about 55, or a hardness of about 6.21 Megapascals (Mpa). In some cases, coating compositions may be selected to provide a relatively elastomeric dried polymer such as a dried polymer having a Shore A hardness of about 80, or a hardness of about 3.45 MPa. In some cases, the first and third dried polymer layers may have a Shore D hardness of 55, or a hardness of 6.21 MPa, and the second layer may have a Shore A hardness of 80, or a hardness of 3.45 MPa.

Although in some cases described above, three polymer layers were employed, it will be appreciated that a greater or lesser number of layers may be employed and that each of the three or more layers may include two or more sublayers. In some cases, the plurality of grommets and the fabric can be positioned between the first and second coating layers. In some cases, the plurality of grommets and the fabric can be positioned elsewhere within the tubular seal, e.g., within a layer, or on the radially innermost or radially outermost surface of the tubular seal.

The mandrel **600** of FIG. 6 includes a taper which results in a tubular seal having a slightly smaller diameter proximal end compared to the diameter of the distal end. In some cases, the diameter of the proximal end can include a diameter reduction of about 3% to about 30% as compared to the diameter of the distal end. The taper allows the tubular seal to be removed from the mandrel with relative ease upon completion of the fabrication process. The smaller proximal diameter of the tubular seal tends to cause the proximal projections to lie more firmly against an anchor element of the replacement heart valve. In some cases, the surface of the mandrel may be textured to create a tubular seal with a reduced contact area. In some cases, the mandrel can be textured using a bead blasting process. In combination with the selection of a relatively hard outer layer, a textured seal surface is believed to result in a lower friction surface.

As shown in FIG. 7E, a tubular seal 760 can include a woven or non-woven fabric embedded throughout a polymer or metal matrix structure. In some cases, at least one leaflet of the heart valve can be secured to the tubular seal in a portion of the tubular seal including the woven or non-woven fabric to minimize blood leakage between the tubular seal and the leaflets.

In some cases, the matrix structure can be made of elastomeric material. In some cases, tubular seal 760 can be made of the fabric alone. The fabric can include non-elastic fibers arranged to allow for the tubular seal 760 to stretch in axial and/or radial directions relative to the axis of the tubular seal 760. In some cases, the non-elastic fibers can be arranged within the tubular member 760 to form an angle of about 45 degrees with the axis of the tubular seal. In some cases, the fabric can be a knit fabric arranged to allow for a predetermined amount of stretch in the axial and/or radial directions. In some cases, the fabric can be made of polymeric materials that include, but are not limited to, polyesters, polyolefins such as polyethylene and polypropylene, polyamides, nylons, and combinations thereof. In some cases, the fabric can have a thickness ranging from about 0.002 inches to about 0.003 inches (about 40 to about 80 microns). In some cases, the fabric can be woven such that spacings between individual fibers create openings in the fabric that together constitutes from about 20% to about 40% of a fabric surface.

A number of embodiments of the invention have been described. Nevertheless, it will be understood that various modifications may be made without departing from the spirit and scope of the invention. Accordingly, other embodiments are within the scope of the following claims.

What is claimed is:

1. A prosthetic heart valve comprising:
 - an expandable member comprising one or more braided wires, the one or more braided wires comprising a first set of wire segments extended helically in a first direction and a second set of wire segments extended helically in a second direction such that each wire segment of the first set intersects a plurality of wire segments from the second set at a plurality of intersection points, wherein the one or more braided wires have crowns where the wire segments of the first set connect to wire segments of the second set;
 - a plurality of leaflets being secured within the expandable member; and
 - a tubular seal comprising an elastomeric material, the tubular seal having an inflow edge being secured to bottom inflow edges of the plurality of leaflets and to the expandable member by a plurality of sutures, characterized by the sutures comprising cross stitches formed around both a wire segment of the first set and a wire segment of the second set at one of the intersection points.
2. The prosthetic heart valve of claim 1, wherein each cross stitch is an independently tied off stitch unconnected to other cross stitches.
3. The prosthetic heart valve of claim 1, wherein each cross stitch is attached at an intersection point immediately adjacent a crown at an inflow side of the expandable member.
4. The prosthetic heart valve of claim 1, wherein the plurality of leaflets are secured together along side edges thereof.
5. The prosthetic heart valve of claim 4, wherein the plurality of leaflets each comprise two sleeve portions,

wherein the sleeve portions are secured to the expandable member by a plurality of anchor elements.

6. The prosthetic heart valve of claim 1, wherein the tubular seal comprises a plurality of non-elastic fibers retained within a matrix of the elastomeric material, the non-elastic fibers being arranged to allow the tubular seal to stretch in an axial or a radial direction.

7. The prosthetic heart valve of claim 6, wherein the non-elastic fibers are part of a fabric.

8. The prosthetic heart valve of claim 7, wherein the fabric has a thickness ranging from about 40 to about 80 microns.

9. The prosthetic heart valve of claim 7, wherein the fabric is a woven fabric.

10. The prosthetic heart valve of claim 9, wherein the woven fabric comprises fibers in a warp direction and fibers in a waft direction, wherein the fibers in both the warp direction and the waft direction are angled with respect to a central axis of the tubular seal.

11. The prosthetic heart valve of claim 10, wherein the fibers in both the warp direction and the waft direction are angled at an angle between 5 degrees and 70 degrees with respect to the central axis of the tubular seal.

12. The prosthetic heart valve of claim 7, wherein the fibers are made of polyester.

13. The prosthetic heart valve of claim 6, wherein the non-elastic fibers are uniformly dispersed throughout the matrix.

14. The prosthetic heart valve of claim 1, wherein the tubular seal has a substantially uniform thickness.

15. A prosthetic heart valve comprising:

- an expandable member comprising one or more braided wires, the one or more braided wires comprising a first set of wire segments and a second set of wire segments such that each wire segment of the first set intersects a plurality of wire segments from the second set at a plurality of intersection points;
- a plurality of leaflets being secured within the expandable member; and
- a tubular seal comprising an elastomeric material, the tubular seal having an inflow edge being secured to bottom inflow edges of the plurality of leaflets and to the expandable member by a plurality of sutures, wherein the sutures comprise cross stitches formed around both a wire segment of the first set and a wire segment of the second set at one of the intersection points;

 wherein the tubular seal comprises an outflow end region and an inflow end region, the inflow end region being a portion of the tubular seal comprising a fabric within a matrix of an elastomeric matrix, wherein the fabric has a non-linear edge defining an interface between the inflow end region and the outflow end region.

16. The prosthetic heart valve of claim 15, wherein the non-linear edge of the fabric has a sinusoidal or scalloped shape.

17. The prosthetic heart valve of claim 15, wherein the plurality of leaflets are secured to the tubular seal by a continuous circumferential running stitch.

18. The prosthetic heart valve of claim 15, wherein the first set of wire segments extends helically in a first direction and a second set of wire segments extends helically in a second direction.

19. The prosthetic heart valve of claim 18, wherein the one or more braided wires have crowns where the wire segments of the first set connect to wire segments of the second set.