



US009820742B2

(12) **United States Patent**  
**Covach et al.**

(10) **Patent No.:** **US 9,820,742 B2**  
(45) **Date of Patent:** **Nov. 21, 2017**

(54) **SURGICAL STAPLER WITH EXPANDABLE JAW**

(71) Applicant: **Applied Medical Resources Corporation**, Rancho Santa Margarita, CA (US)

(72) Inventors: **Jonathan Covach**, Rancho Santa Margarita, CA (US); **Matthew M. Becerra**, Rancho Santa Margarita, CA (US); **Gary M. Johnson**, Rancho Santa Margarita, CA (US)

(73) Assignee: **Applied Medical Resources Corporation**, Rancho Santa Margarita, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 803 days.

(21) Appl. No.: **14/211,570**

(22) Filed: **Mar. 14, 2014**

(65) **Prior Publication Data**

US 2014/0263540 A1 Sep. 18, 2014

**Related U.S. Application Data**

(60) Provisional application No. 61/793,065, filed on Mar. 15, 2013.

(51) **Int. Cl.**

*A61B 17/068* (2006.01)  
*A61B 17/072* (2006.01)  
*A61B 17/00* (2006.01)

(52) **U.S. Cl.**

CPC *A61B 17/07207* (2013.01); *A61B 2017/0046* (2013.01); *A61B 2017/00477* (2013.01); *A61B 2017/07257* (2013.01)

(58) **Field of Classification Search**

CPC .... *A61B 17/07207*; *A61B 2017/07257*; *A61B 2017/00477*; *A61B 2017/0046*

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,494,533 A 2/1970 Green et al.  
4,608,981 A 9/1986 Rothfuss et al.

(Continued)

FOREIGN PATENT DOCUMENTS

RU 2063710 7/1996

OTHER PUBLICATIONS

The International Bureau of WIPO, International Preliminary Report on Patentability, dated Sep. 24, 2015, for International Application No. PCT/US2014/027768.

International Searching Authority, U.S., The International Search Report and the Written Opinion of the International Searching authority for International application PCT/US2014/027768, titled "Surgical Stapler with Expandable Jaw", dated Jul. 25, 2014.

(Continued)

*Primary Examiner* — Thanh Truong


*Assistant Examiner* — Thomas Wittenschlaeger

(74) *Attorney, Agent, or Firm* — John F. Heal

(57) **ABSTRACT**

Jaw assemblies for a surgical stapler are provided. The jaw assemblies comprise a first jaw having a first clamping surface and a plurality of staples disposed therein and second jaw assembly having a second clamping surface. The jaw assemblies can be actuated from a closed configuration in which the first clamping surface contacts or is adjacent to the second clamping surface to an open configuration in which the second jaw is pivoted away from the first jaw to a stapling position in which the second clamping surface is parallel to the first clamping surface and spaced apart from the first clamping surface. A pivoting link or sliding pivot joint can couple the second jaw to the first jaw to facilitate motion between the closed position, the open position, and the stapling position.

**5 Claims, 12 Drawing Sheets**

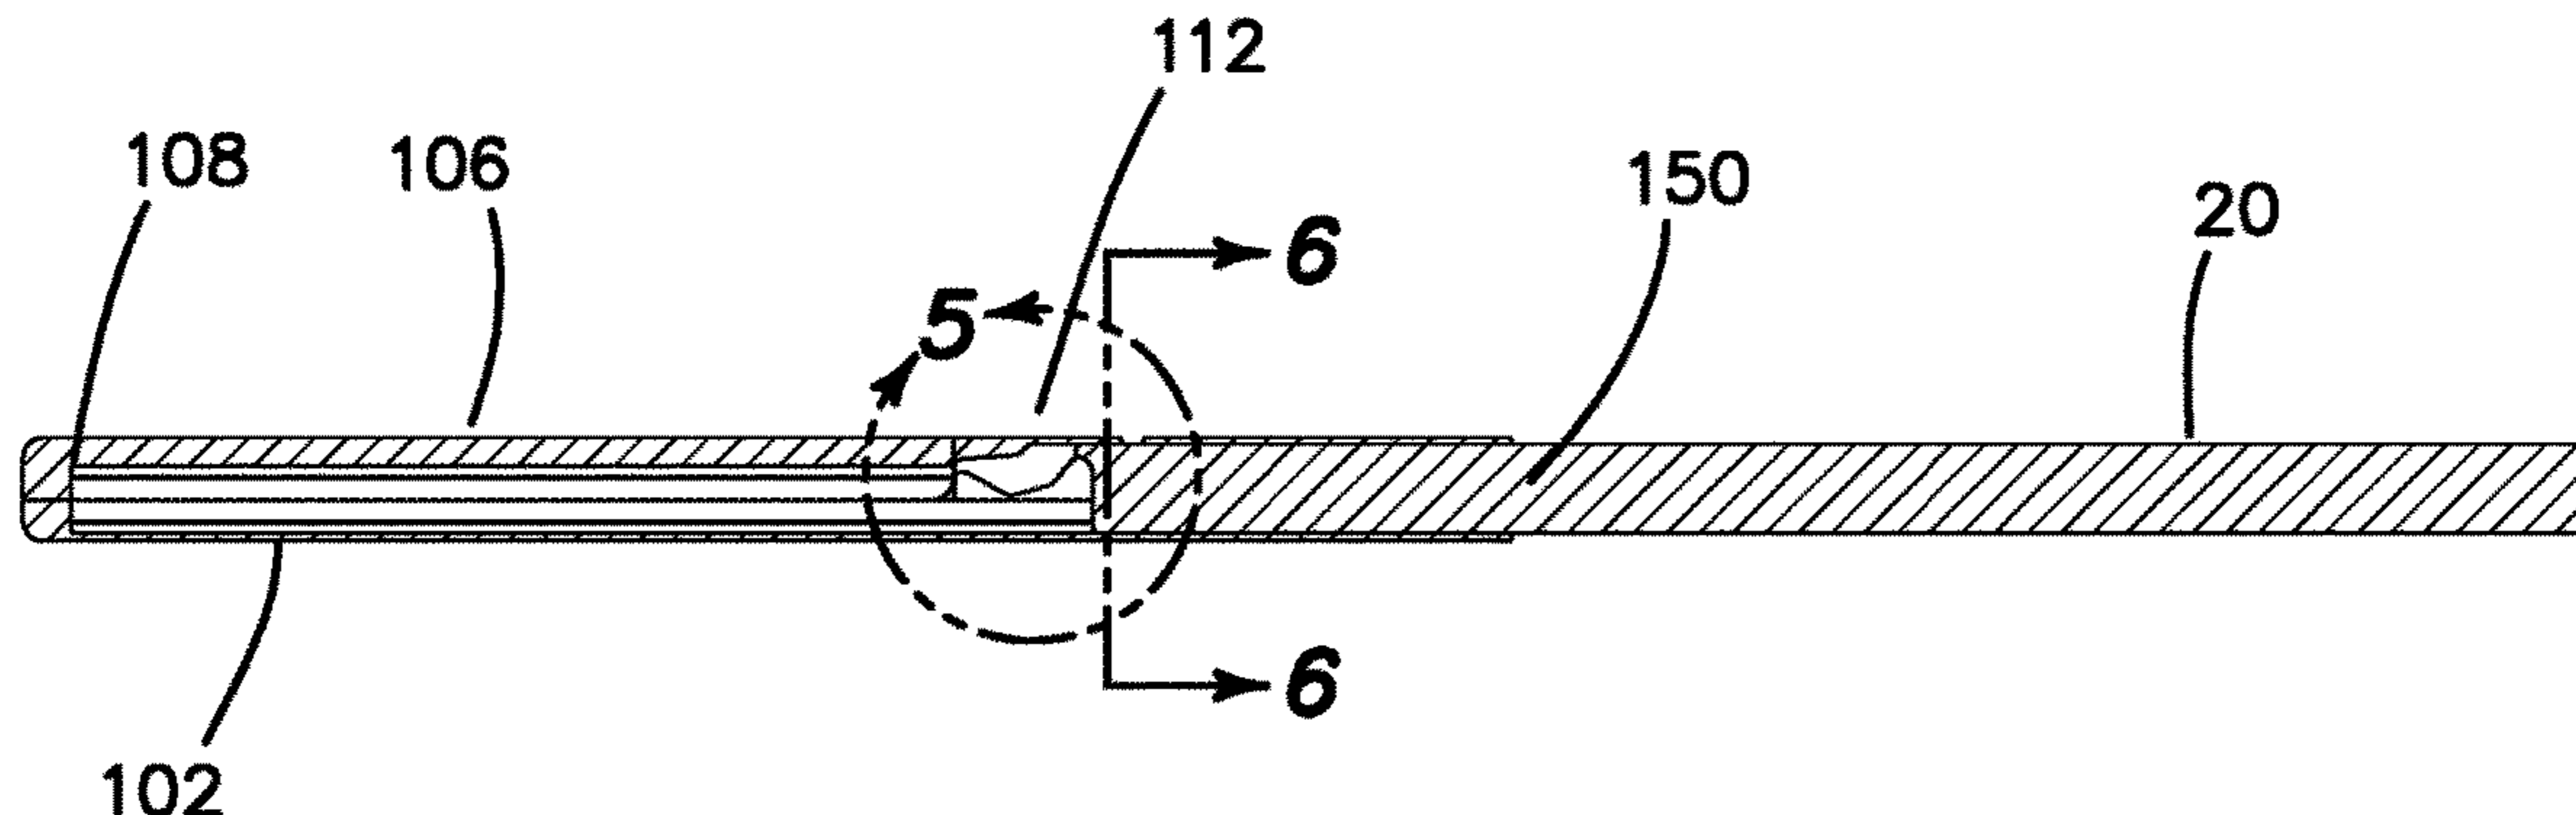

(56)

**References Cited**

U.S. PATENT DOCUMENTS

5,364,001 A \* 11/1994 Bryan ..... A61B 17/07207  
227/175.1  
5,413,268 A \* 5/1995 Green ..... A61B 17/07207  
227/176.1  
5,433,721 A \* 7/1995 Hooven ..... A61B 17/072  
227/175.1  
5,447,265 A 9/1995 Vidal et al.  
5,489,058 A 2/1996 Plyley  
5,697,542 A \* 12/1997 Knodel ..... A61B 17/07207  
227/175.1  
6,716,232 B1 \* 4/2004 Vidal ..... A61B 17/07207  
227/176.1  
7,617,961 B2 \* 11/2009 Viola ..... A61B 17/07207  
227/175.1  
7,651,017 B2 1/2010 Ortiz et al.  
7,845,534 B2 12/2010 Viola et al.  
8,596,513 B2 12/2013 Olson  
2002/0062136 A1 5/2002 Hillstead  
2006/0235442 A1 10/2006 Huitema  
2011/0290851 A1 \* 12/2011 Shelton, IV ..... A61B 17/07207  
227/176.1  
2013/0056521 A1 3/2013 Swensgard  
2013/0240604 A1 9/2013 Knodel

OTHER PUBLICATIONS

European Patent Office, Partial European Search Report for Euro-  
pean Application No. EP 14762896.0, entitled "Surgical Stapler  
With Expandable Jaw," dated Apr. 10, 2017, 6 pgs.

\* cited by examiner

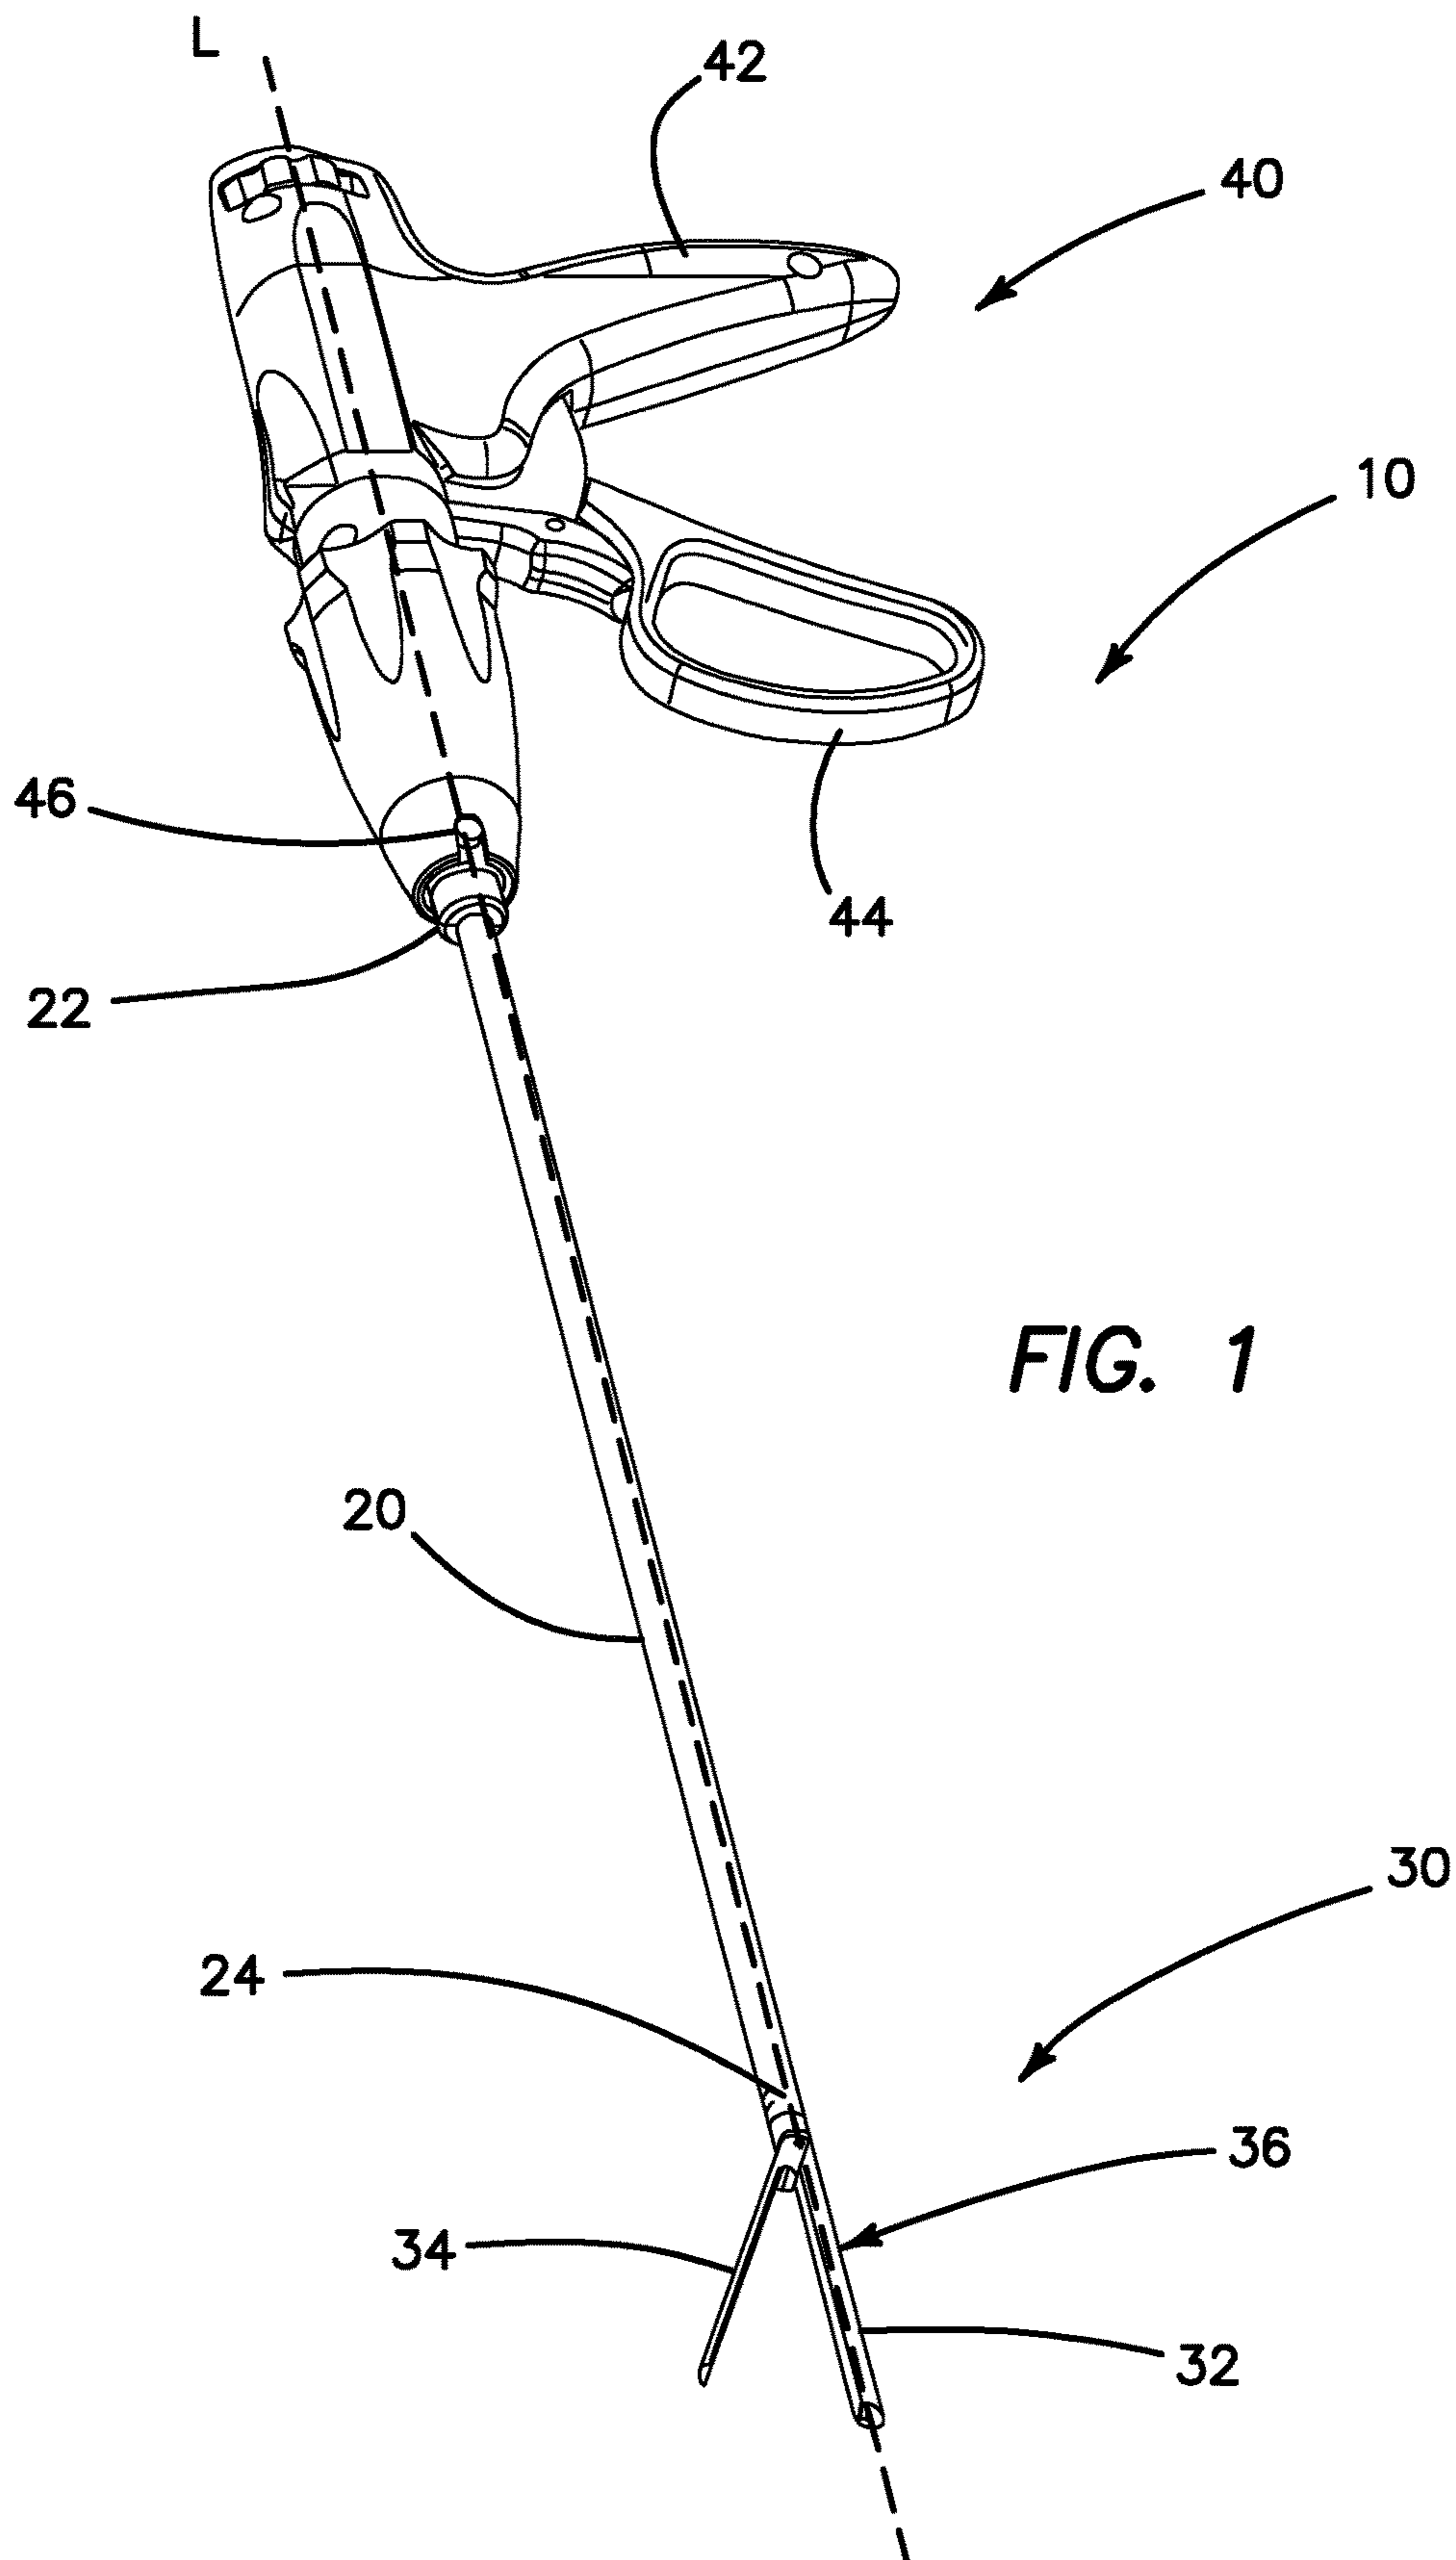


FIG. 1

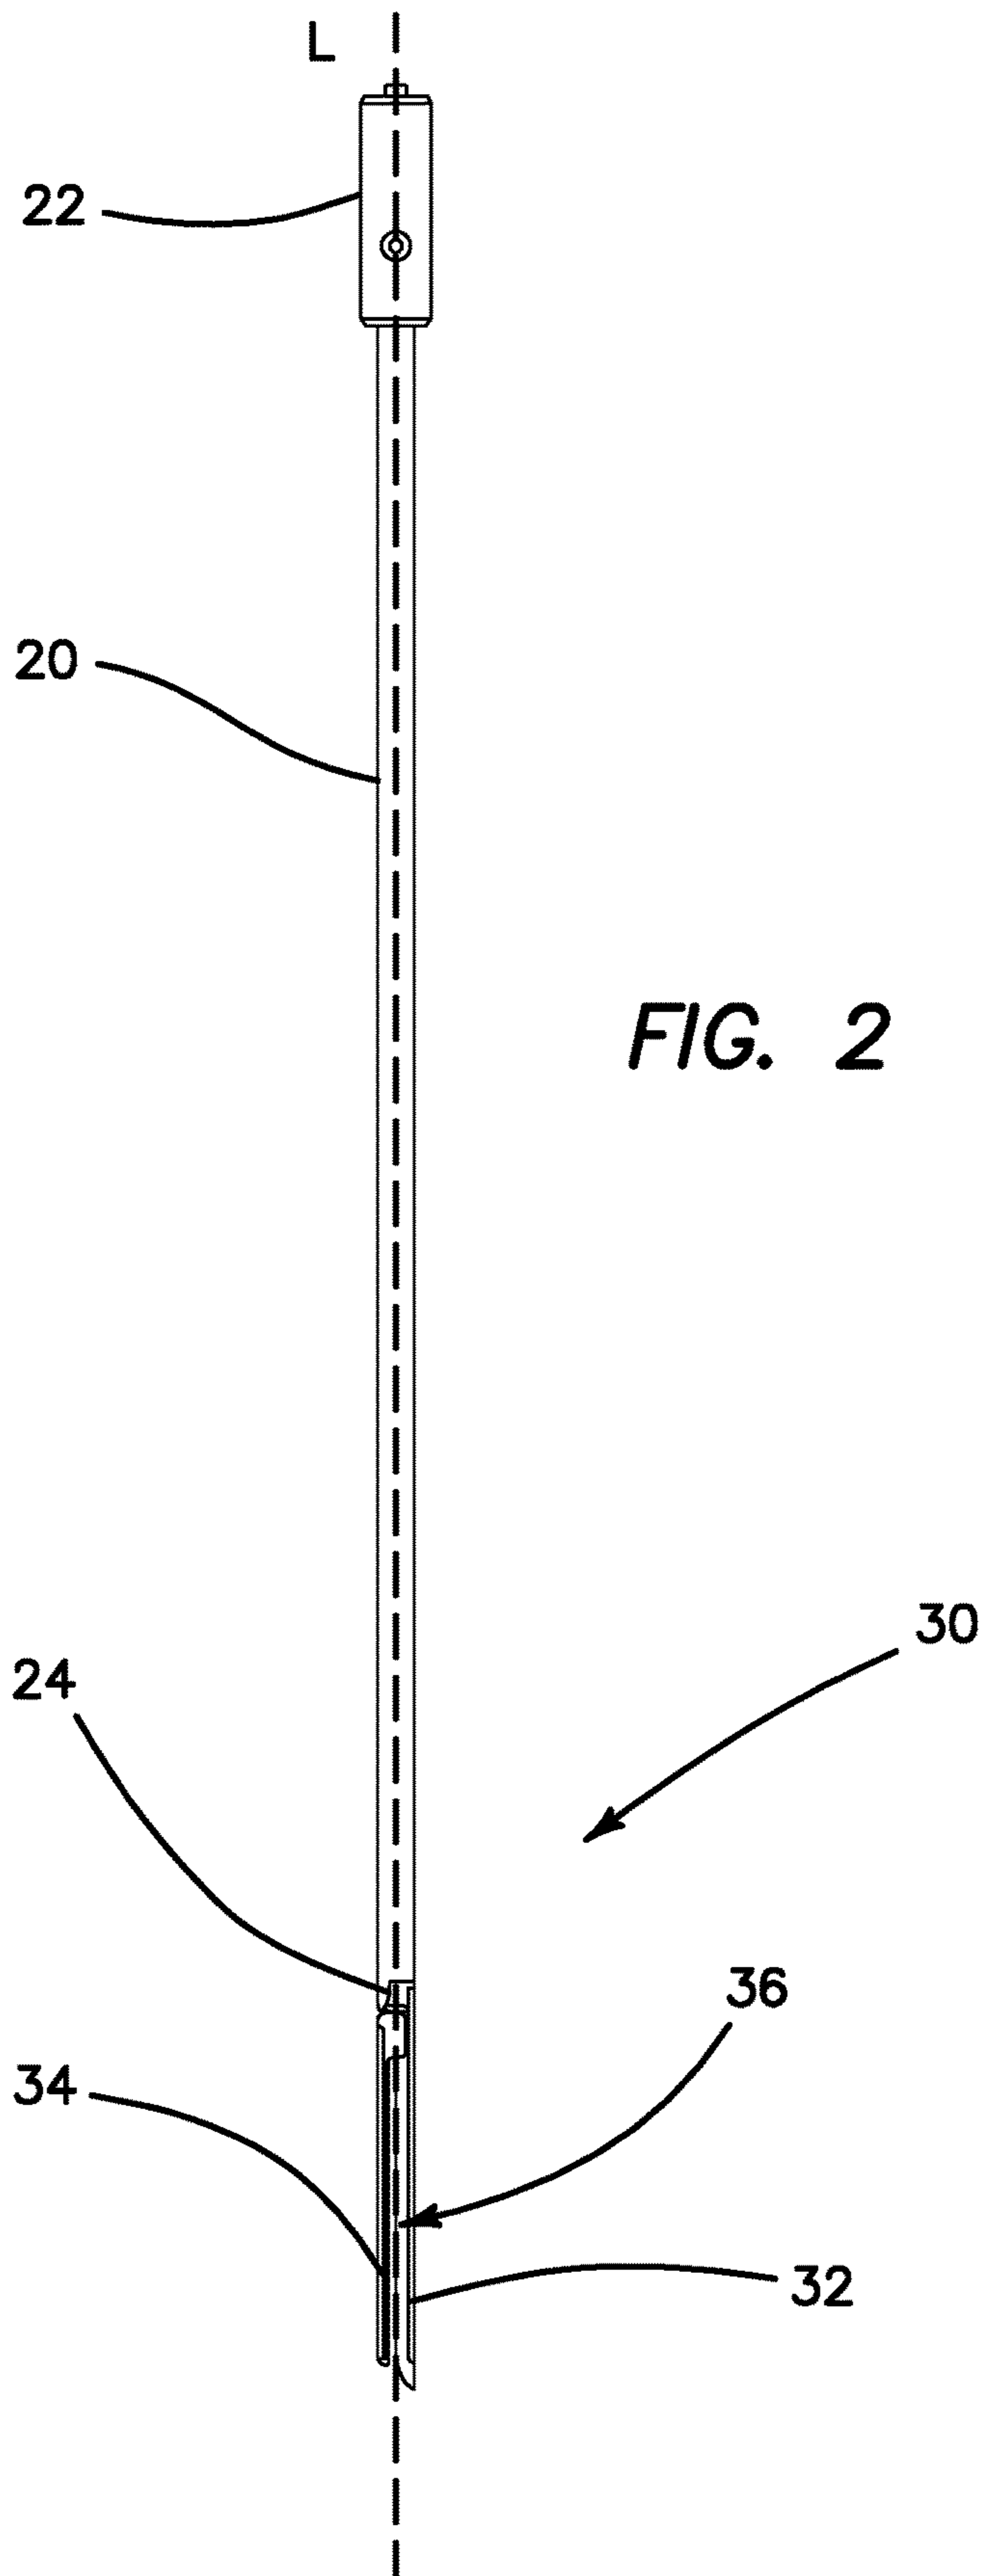
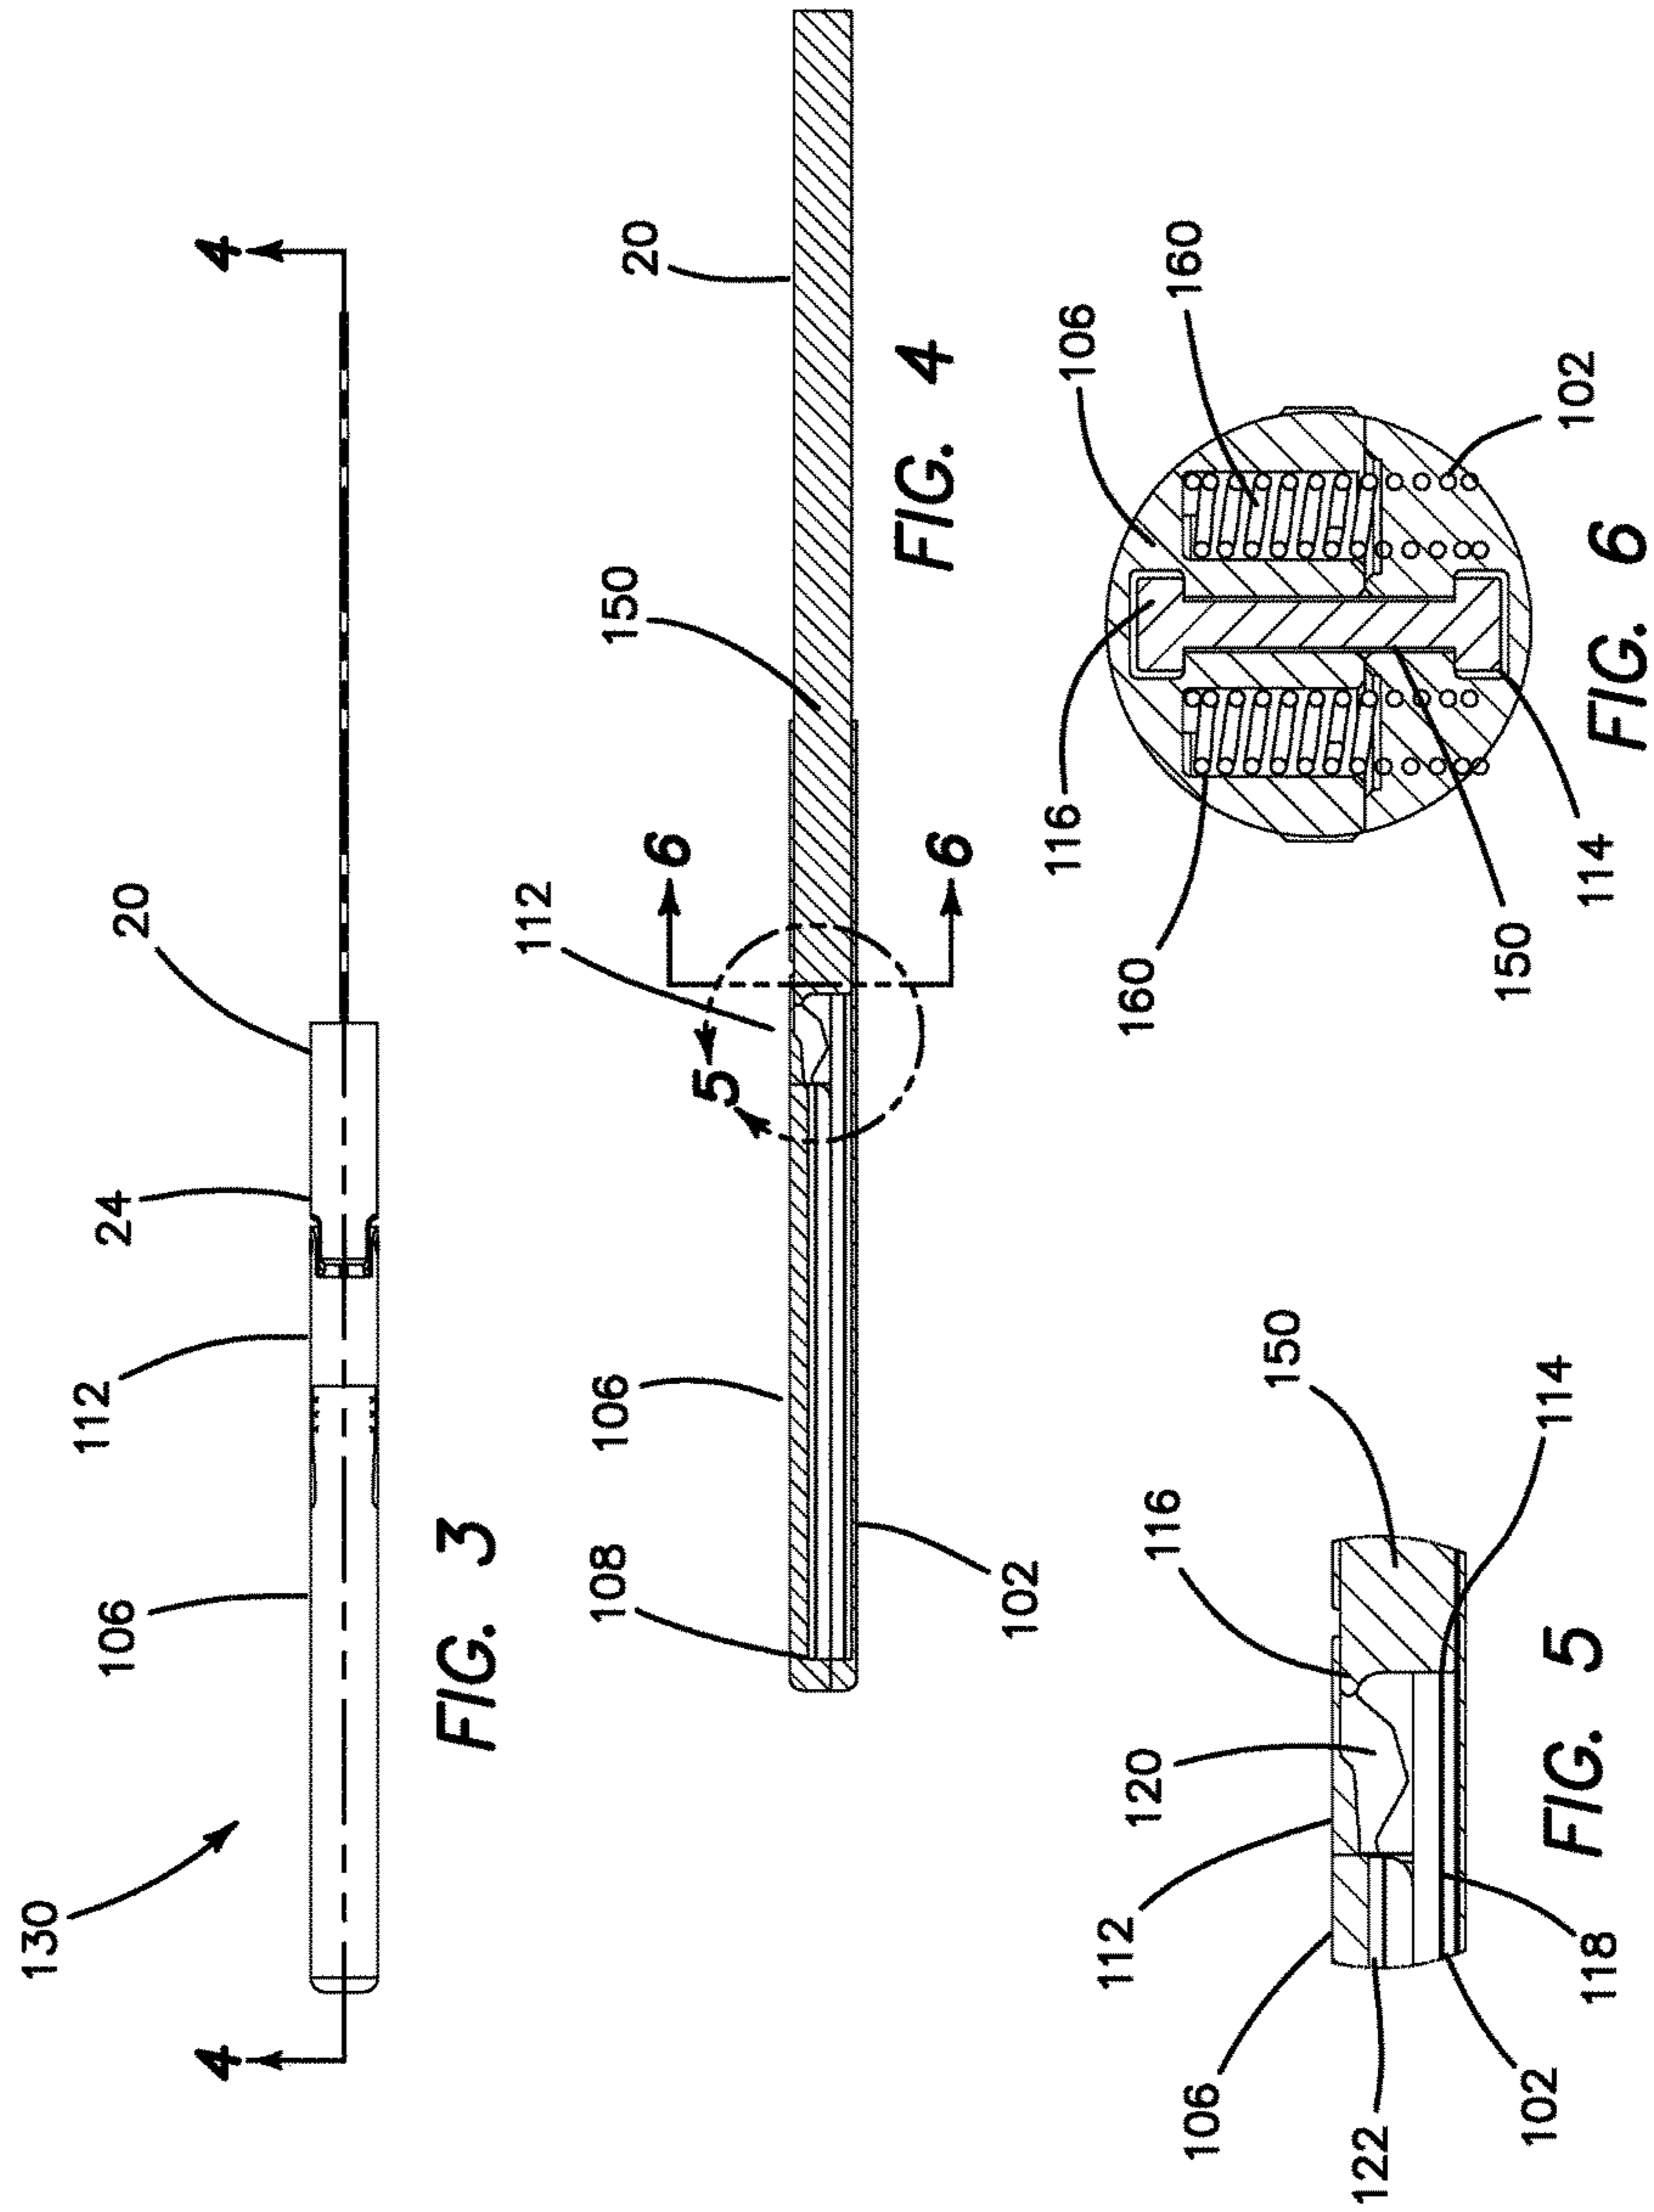
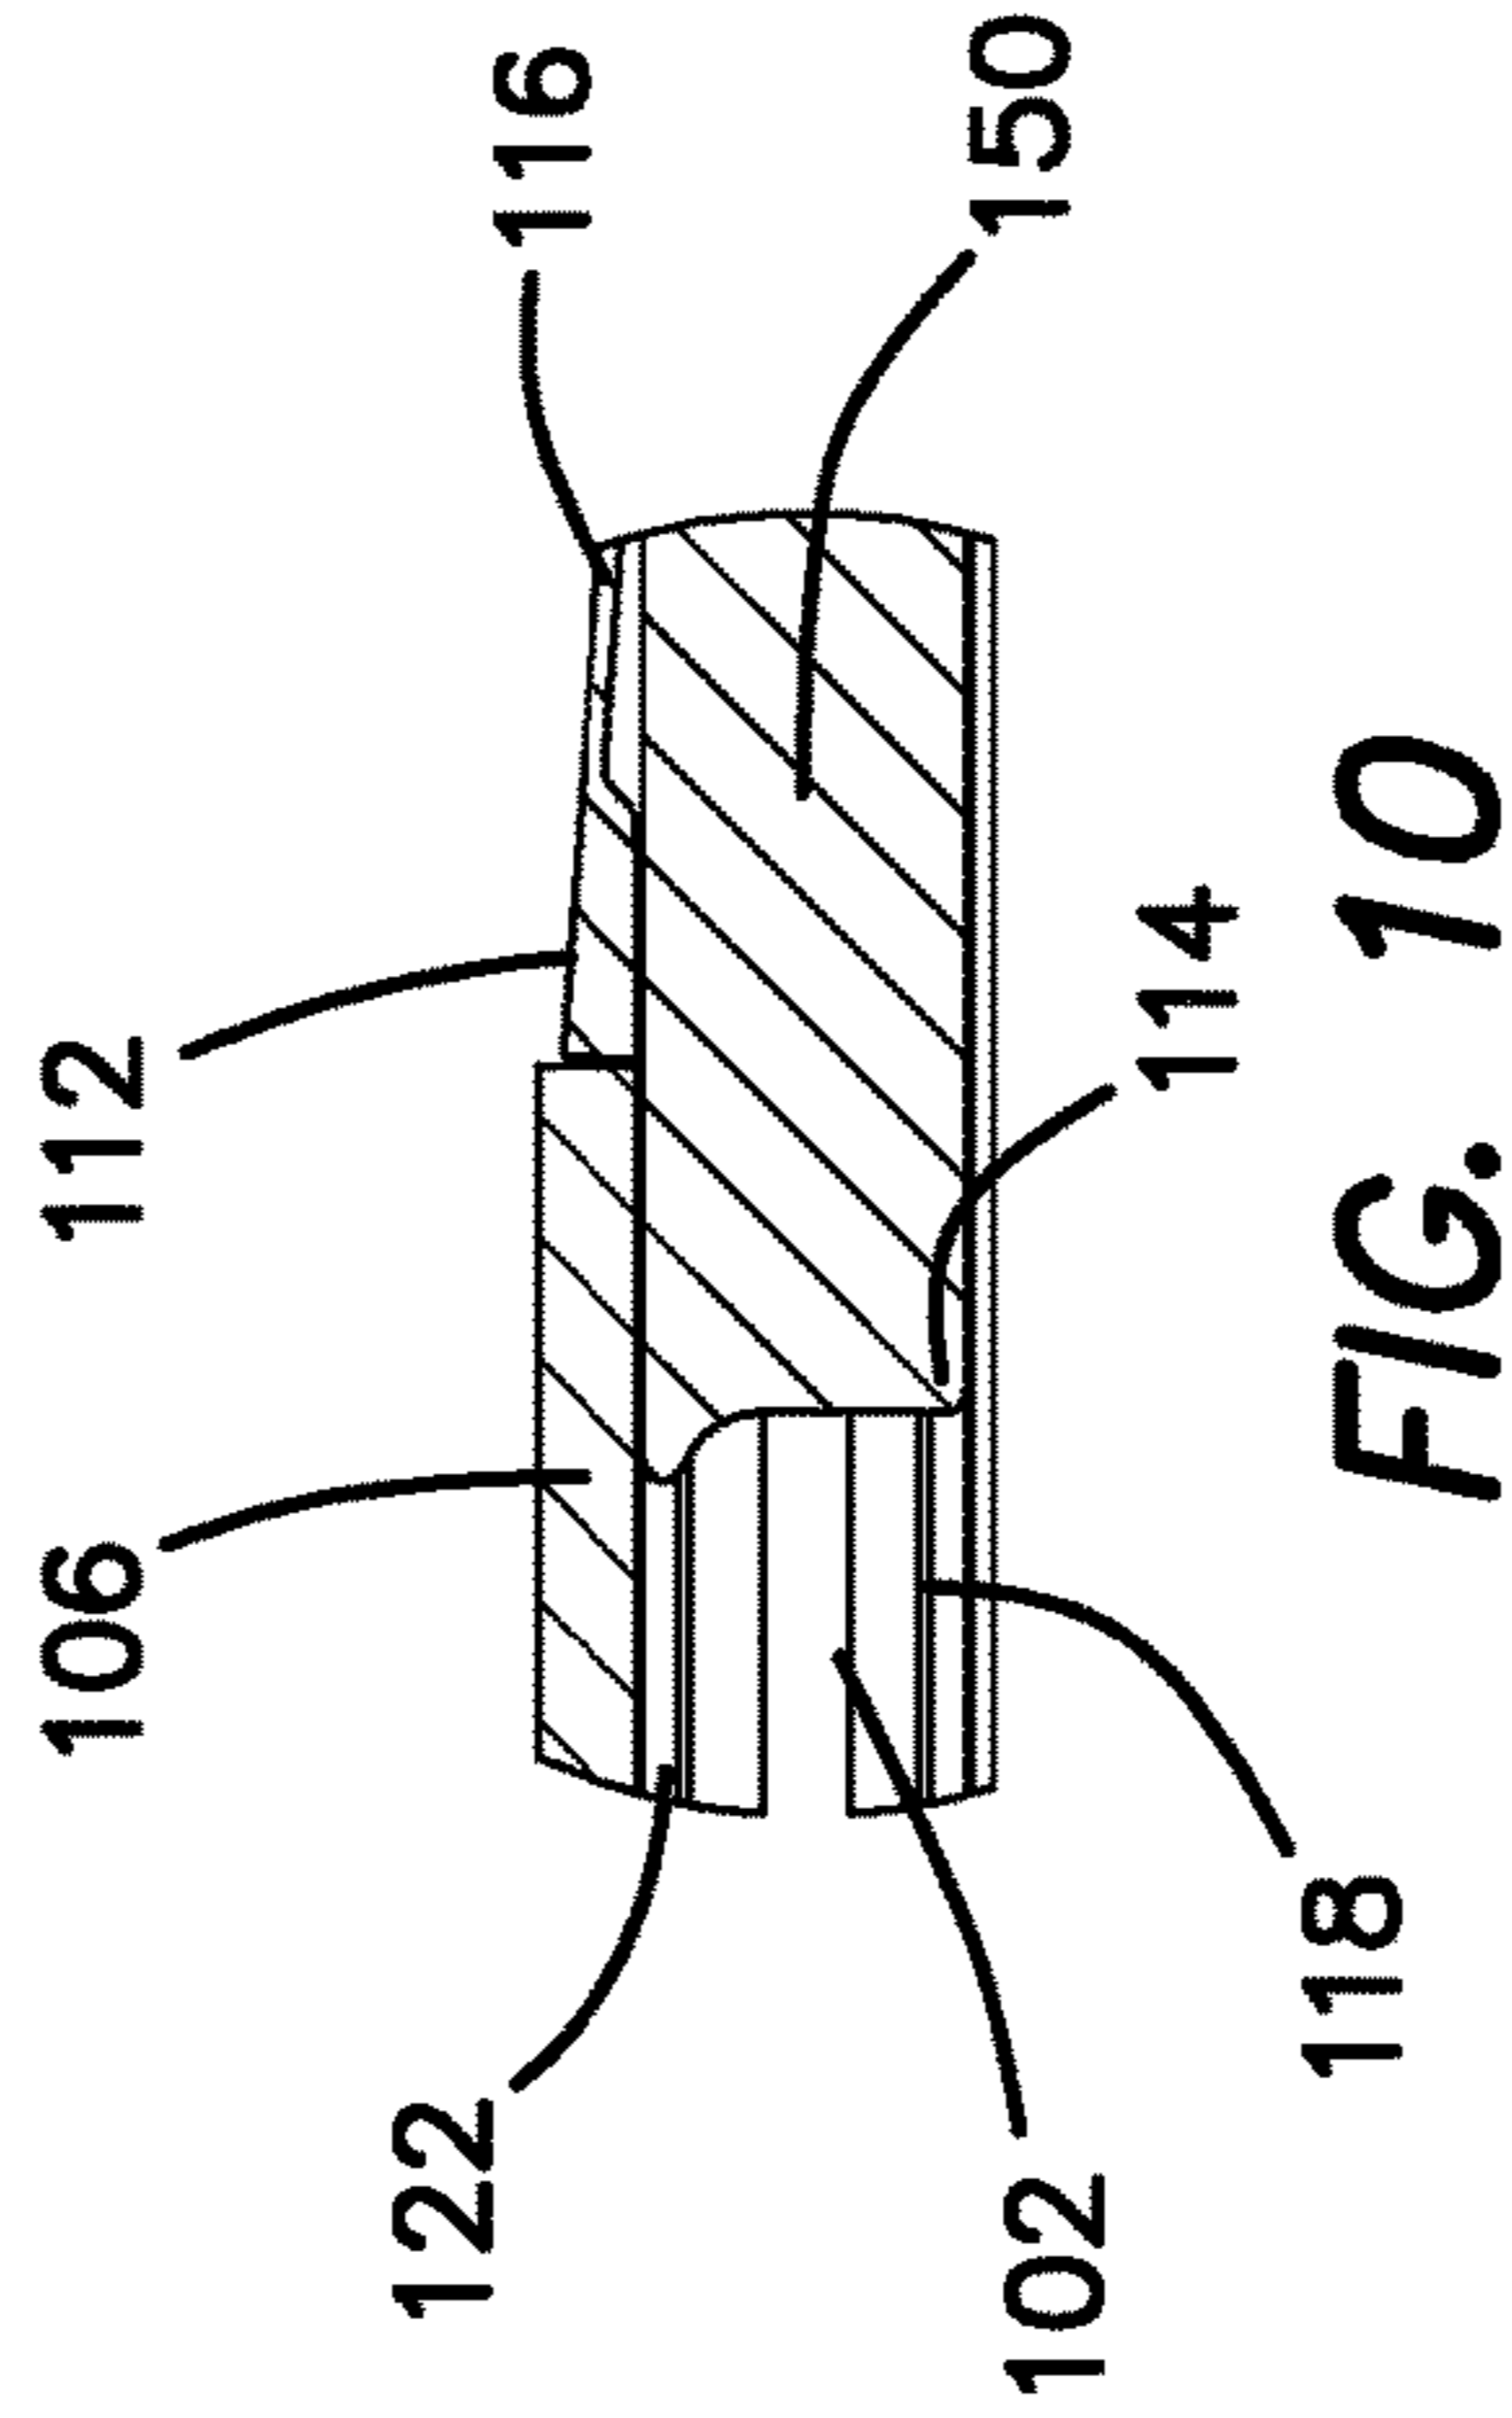
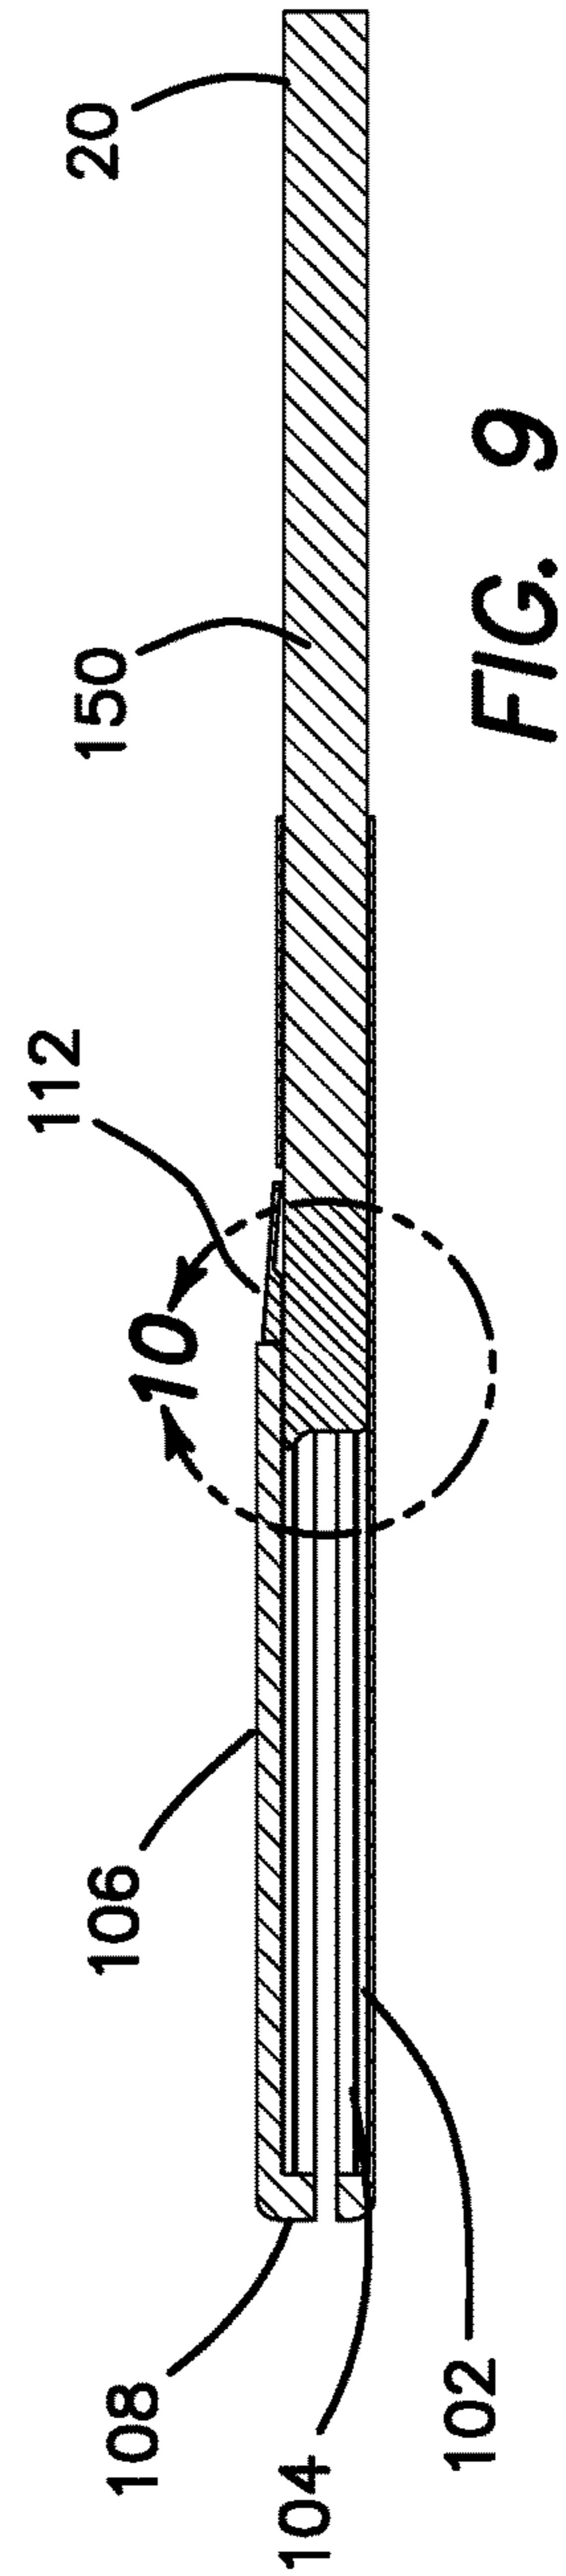
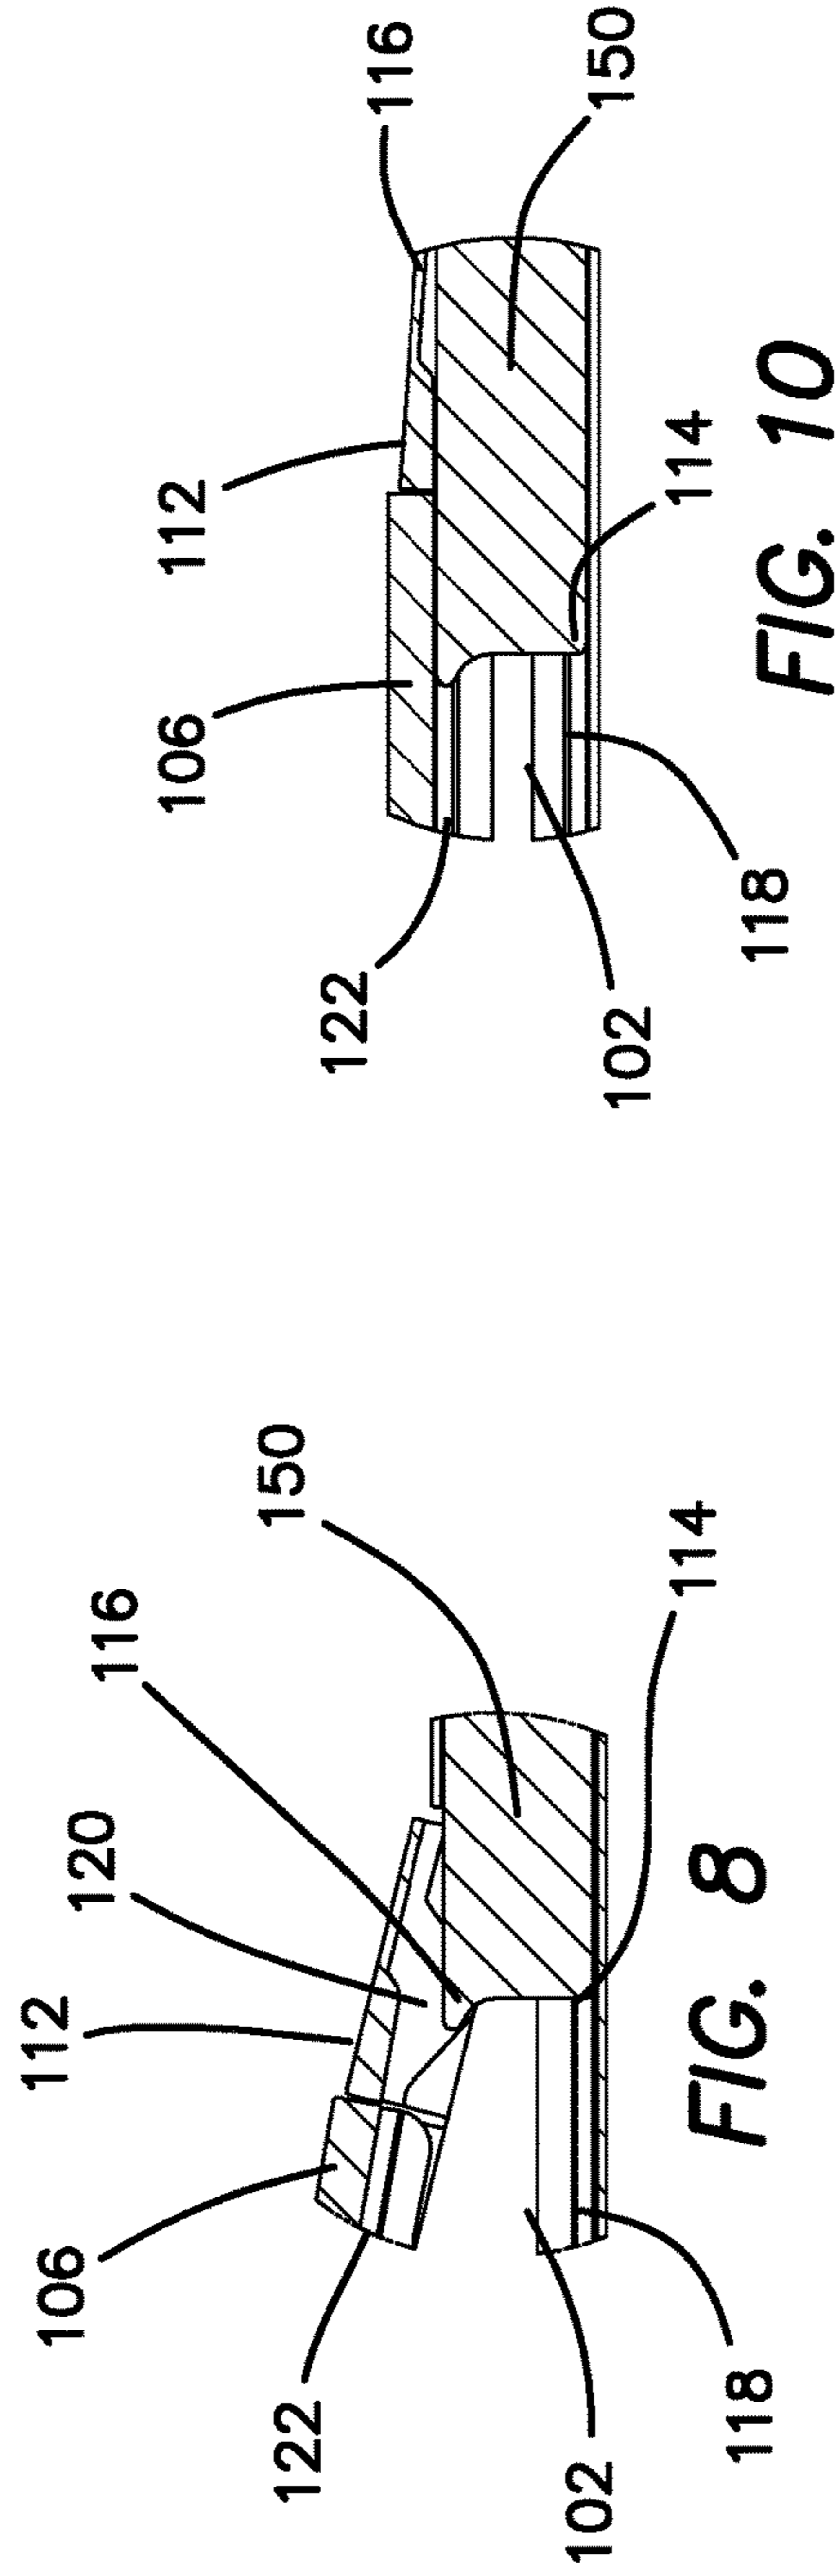
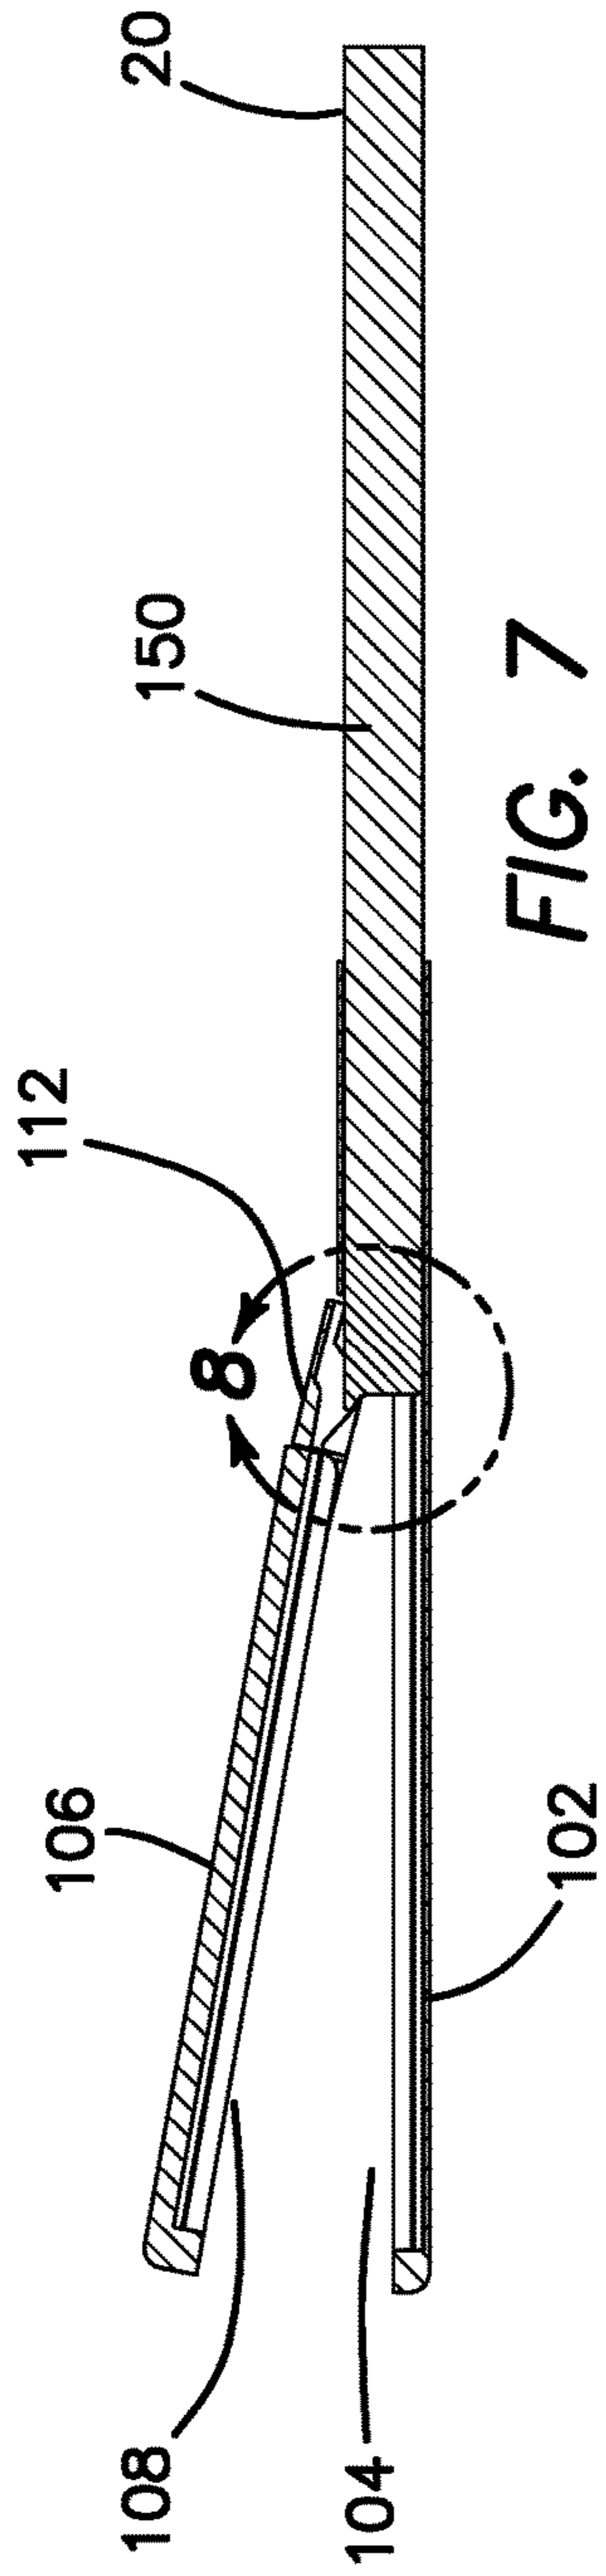


FIG. 2





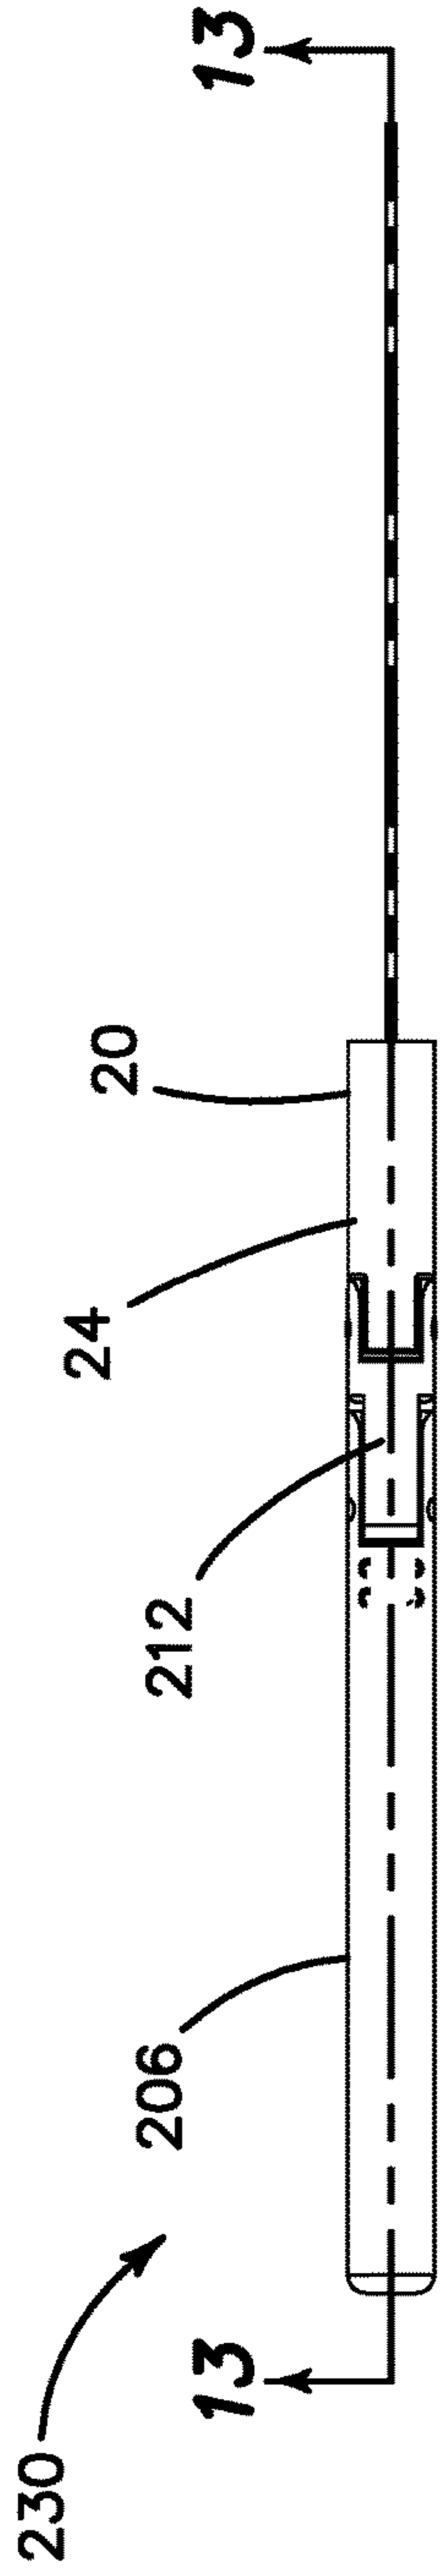


FIG. 11

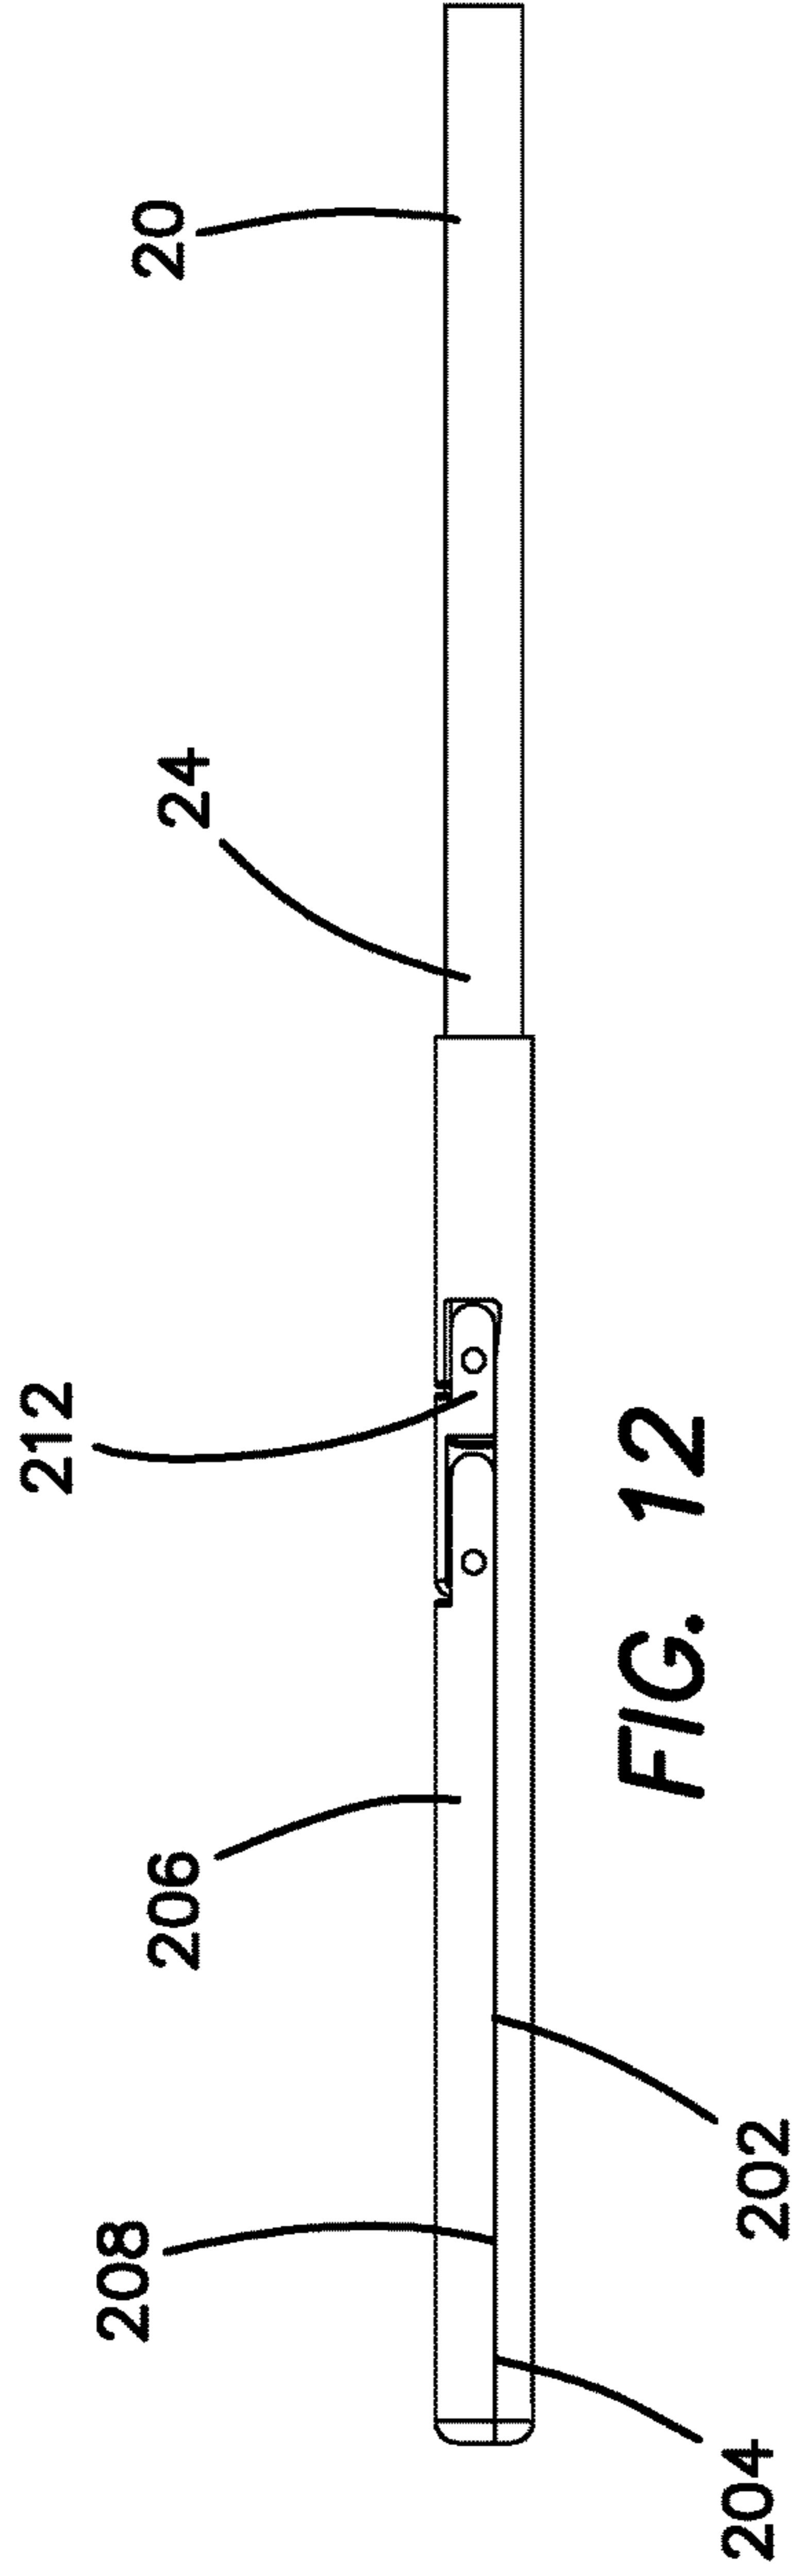


FIG. 12

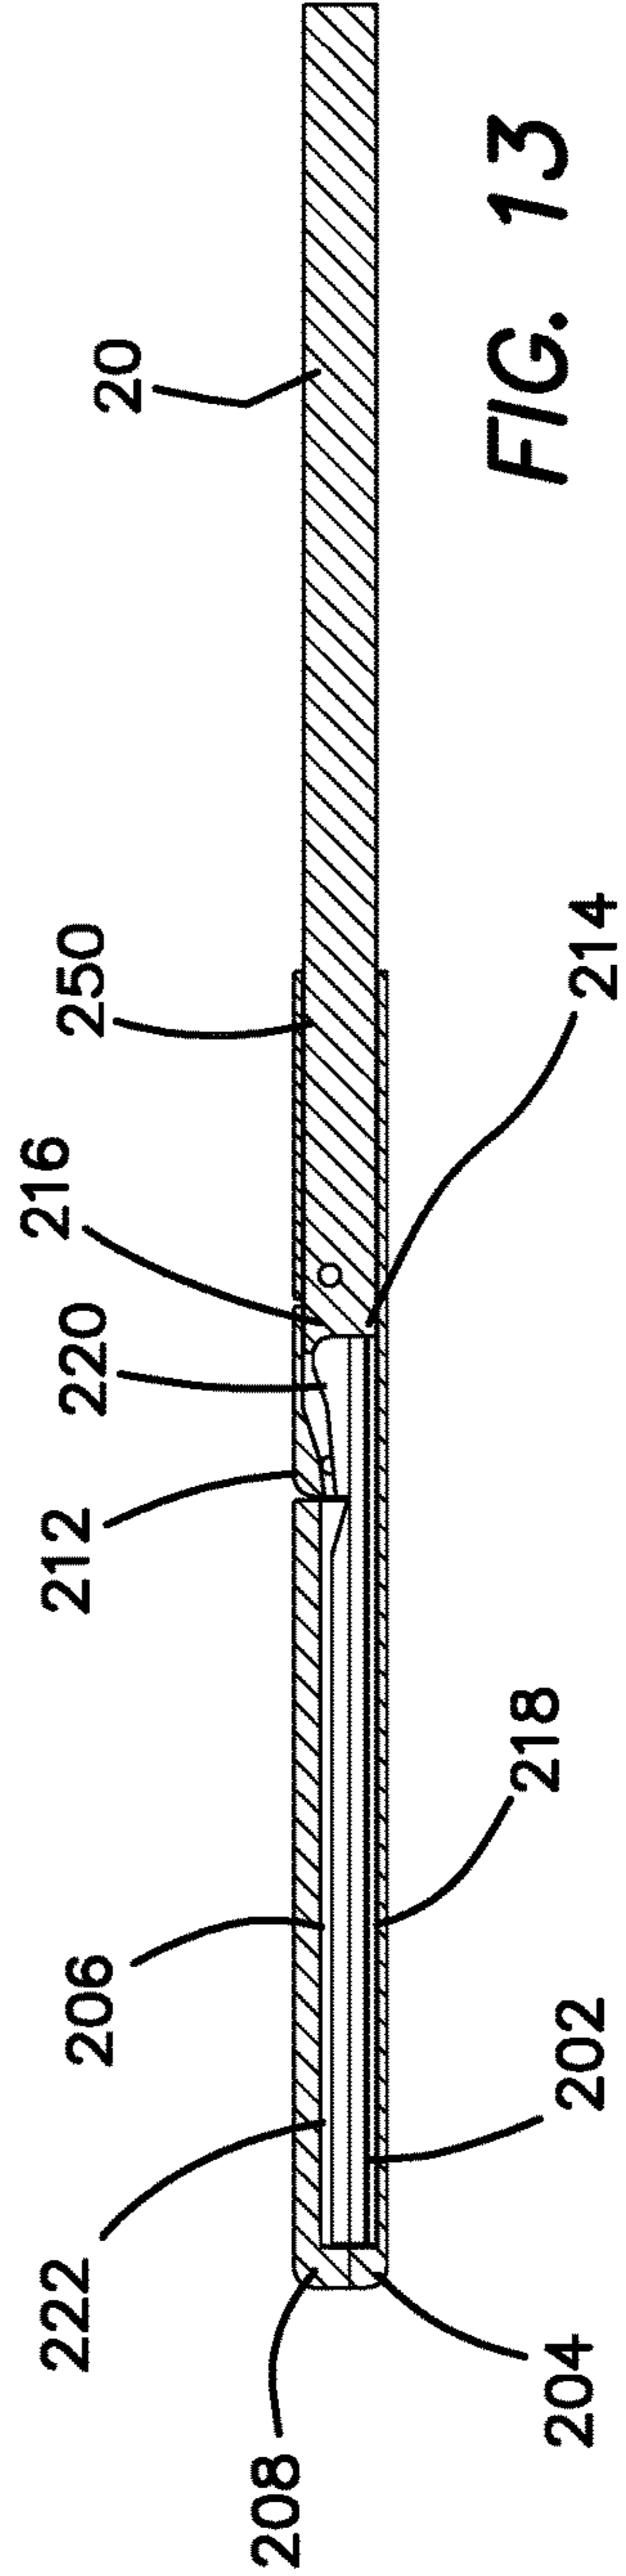
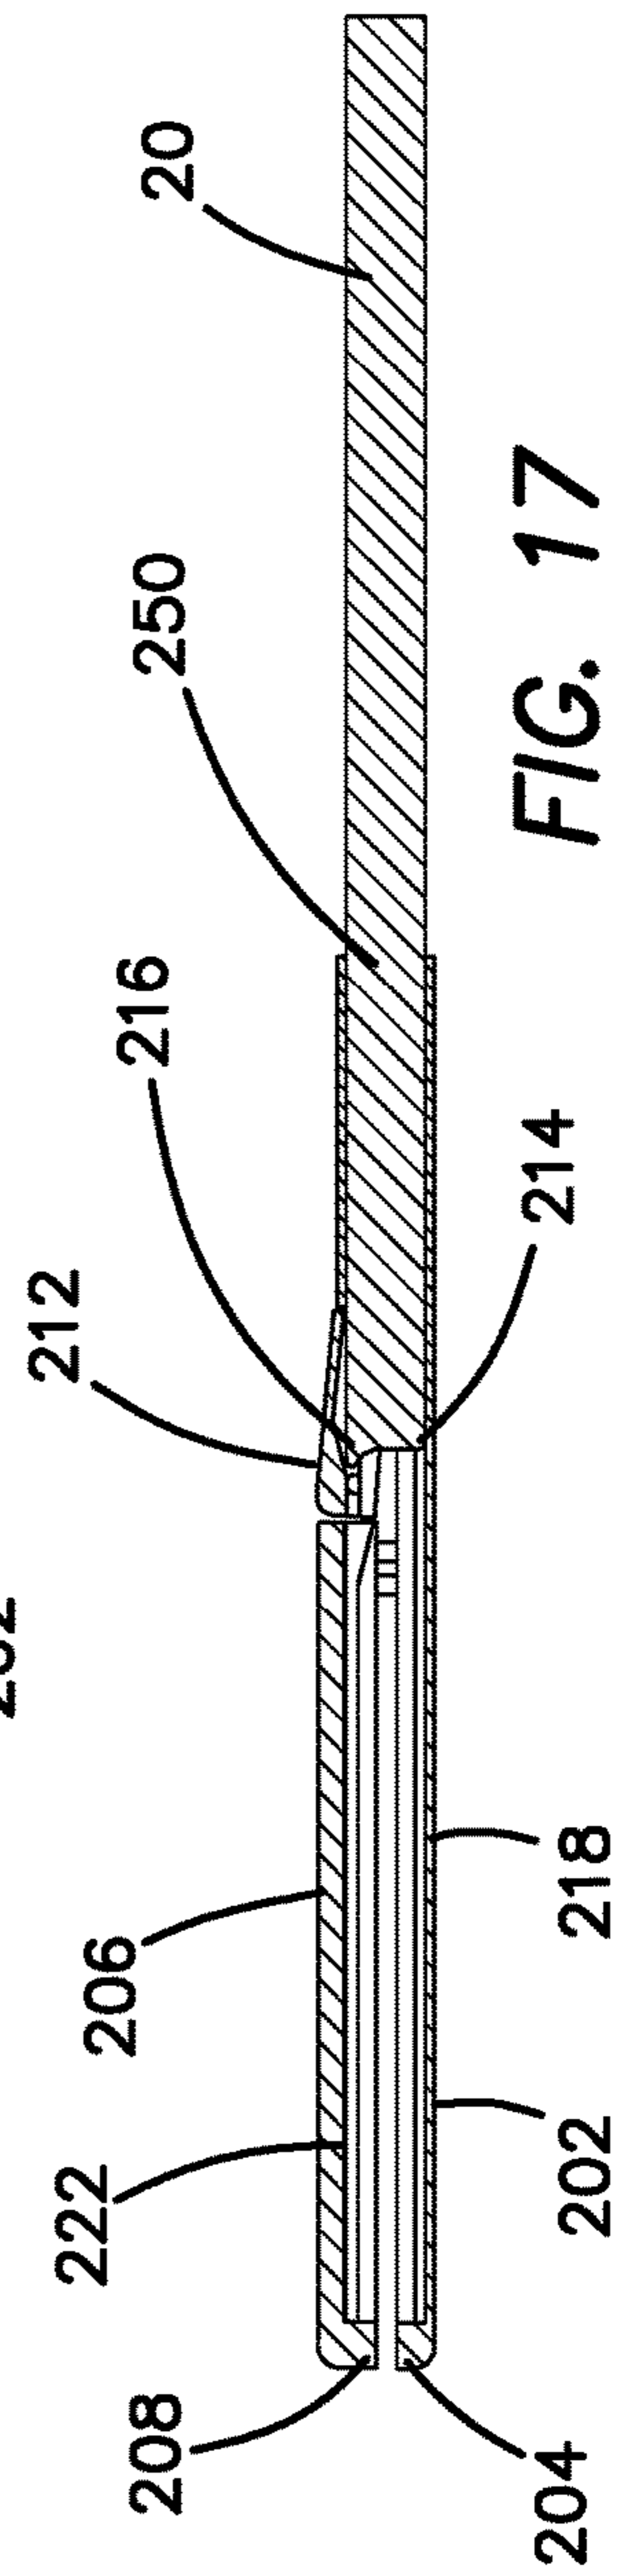
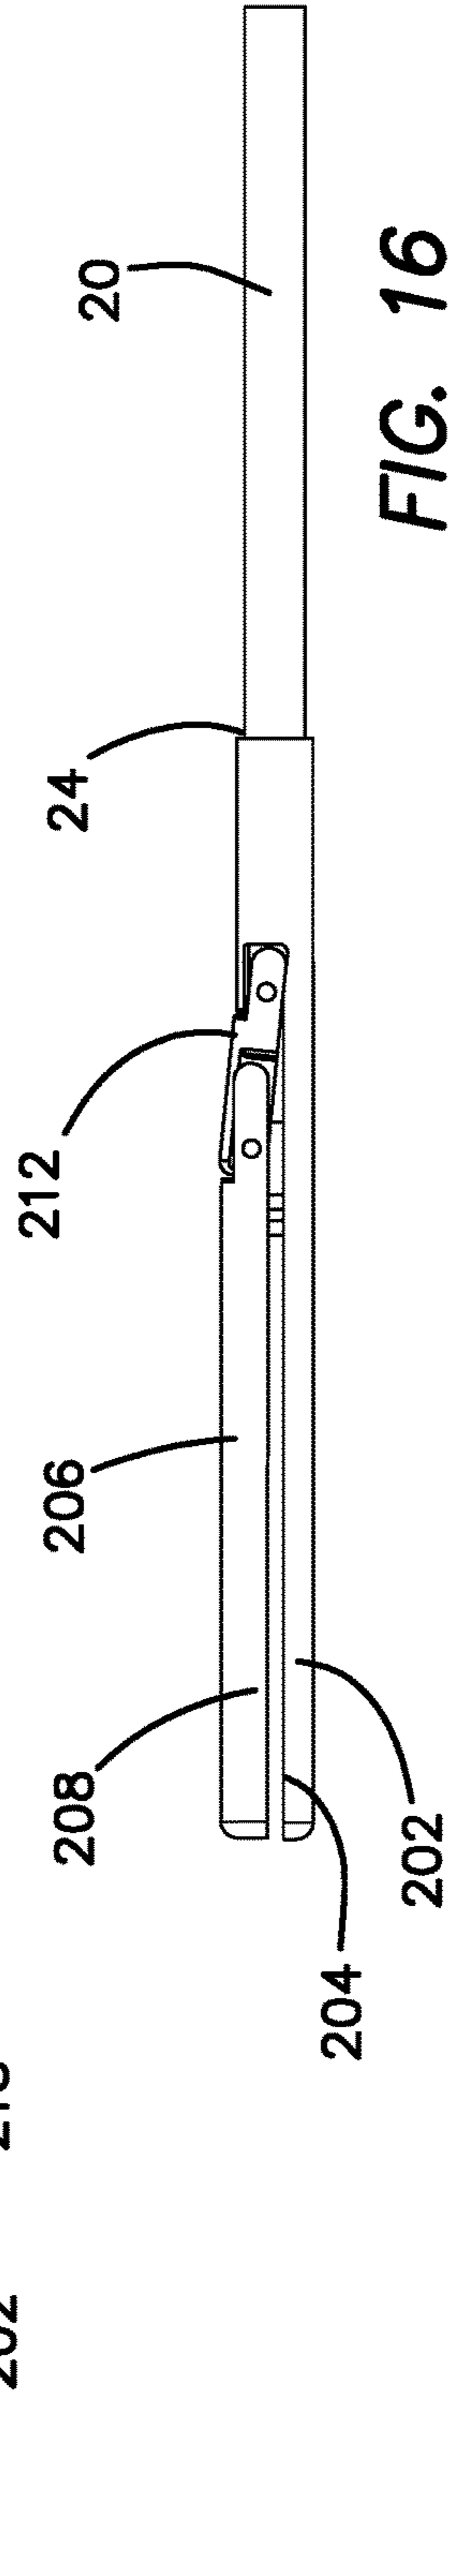
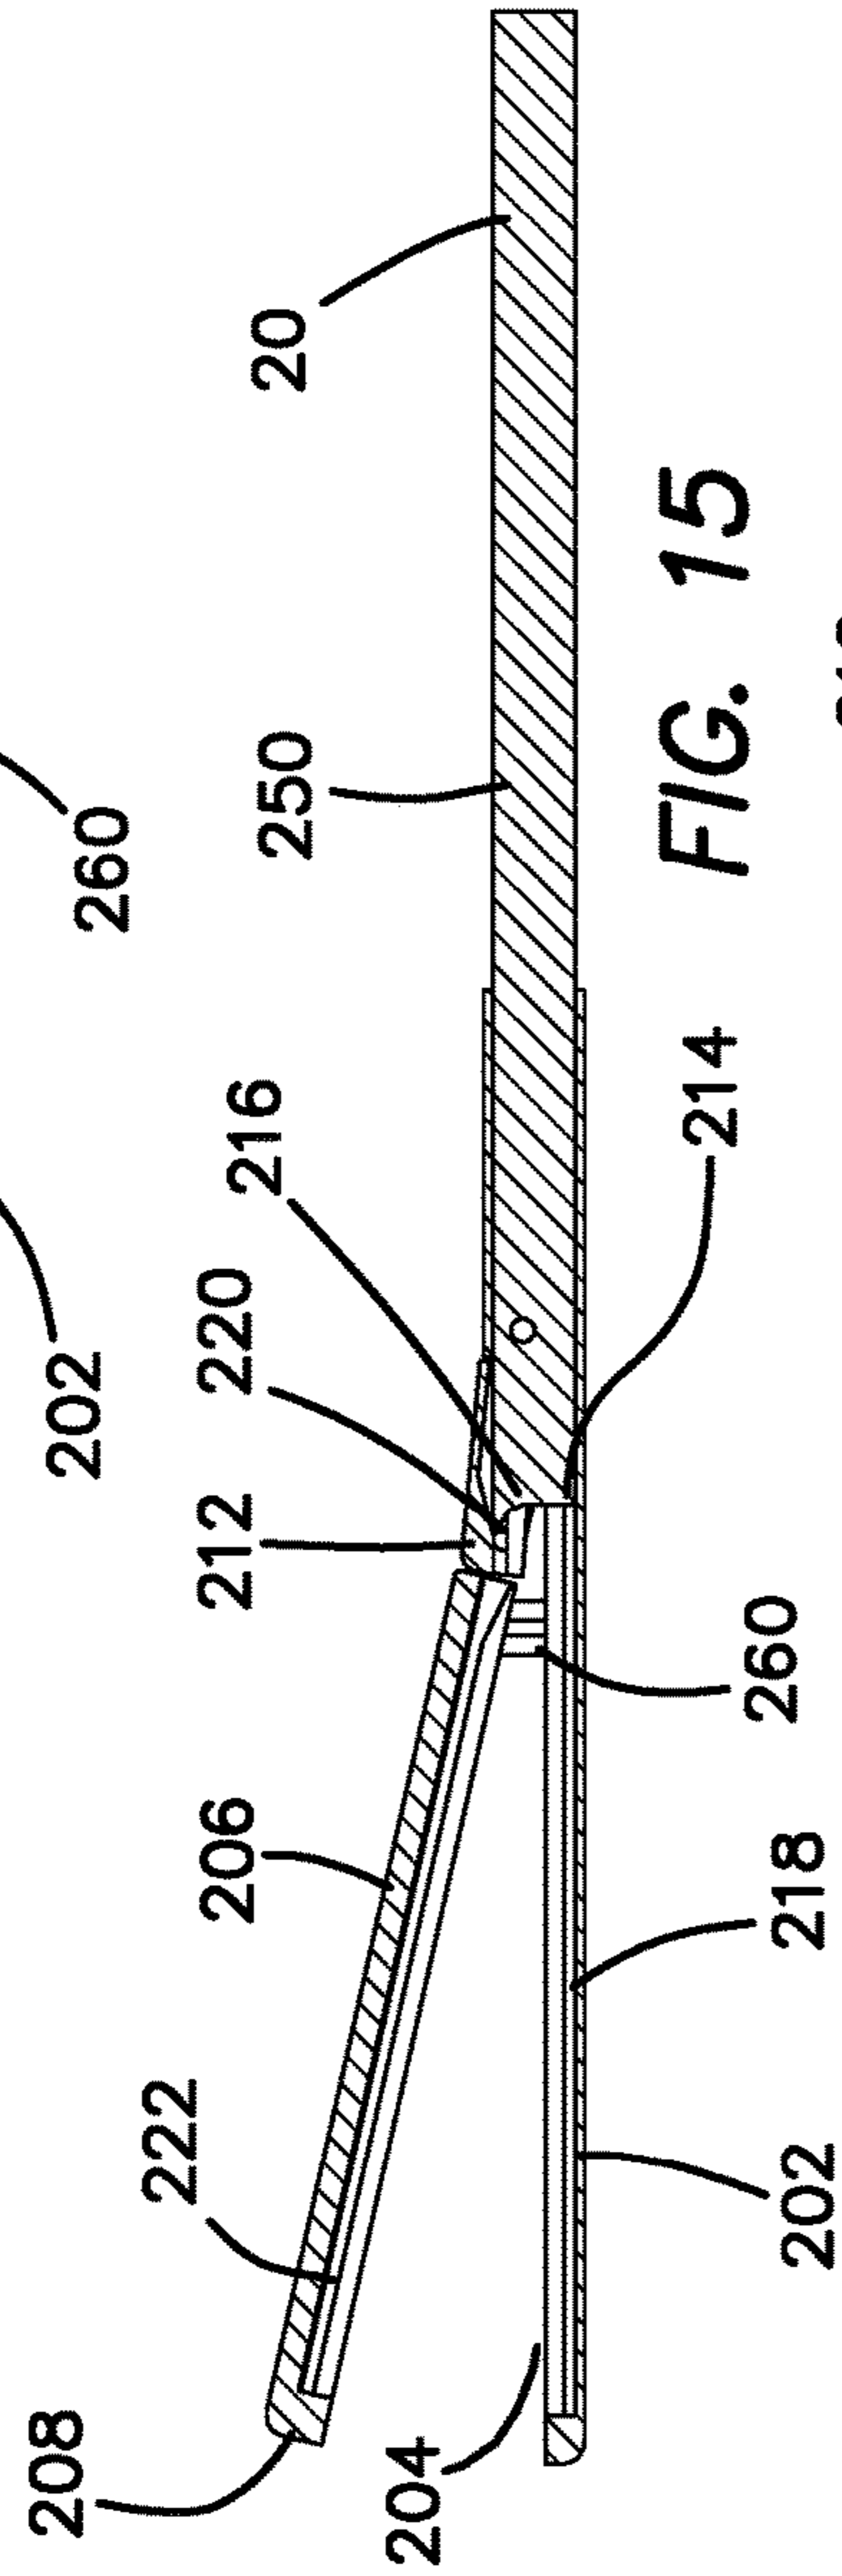
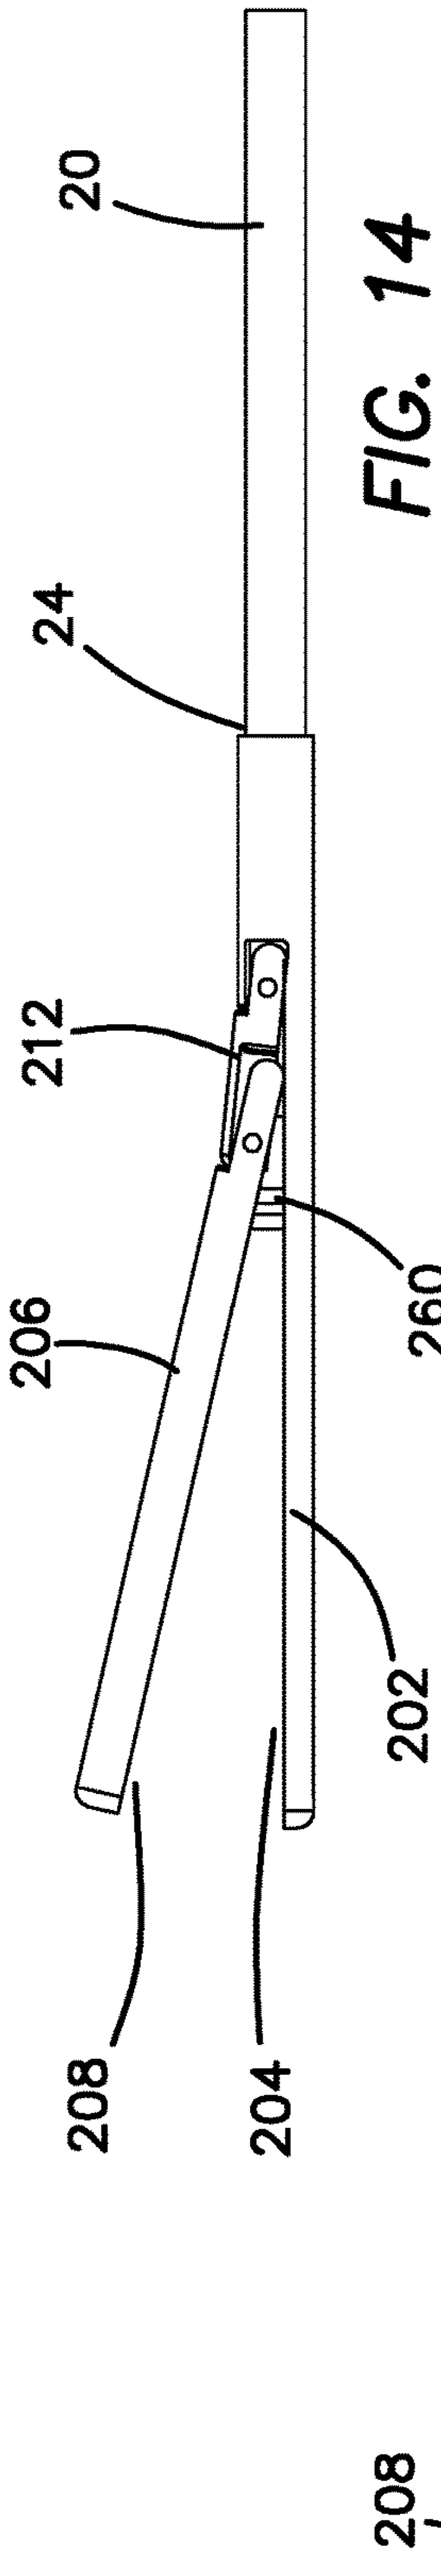


FIG. 13





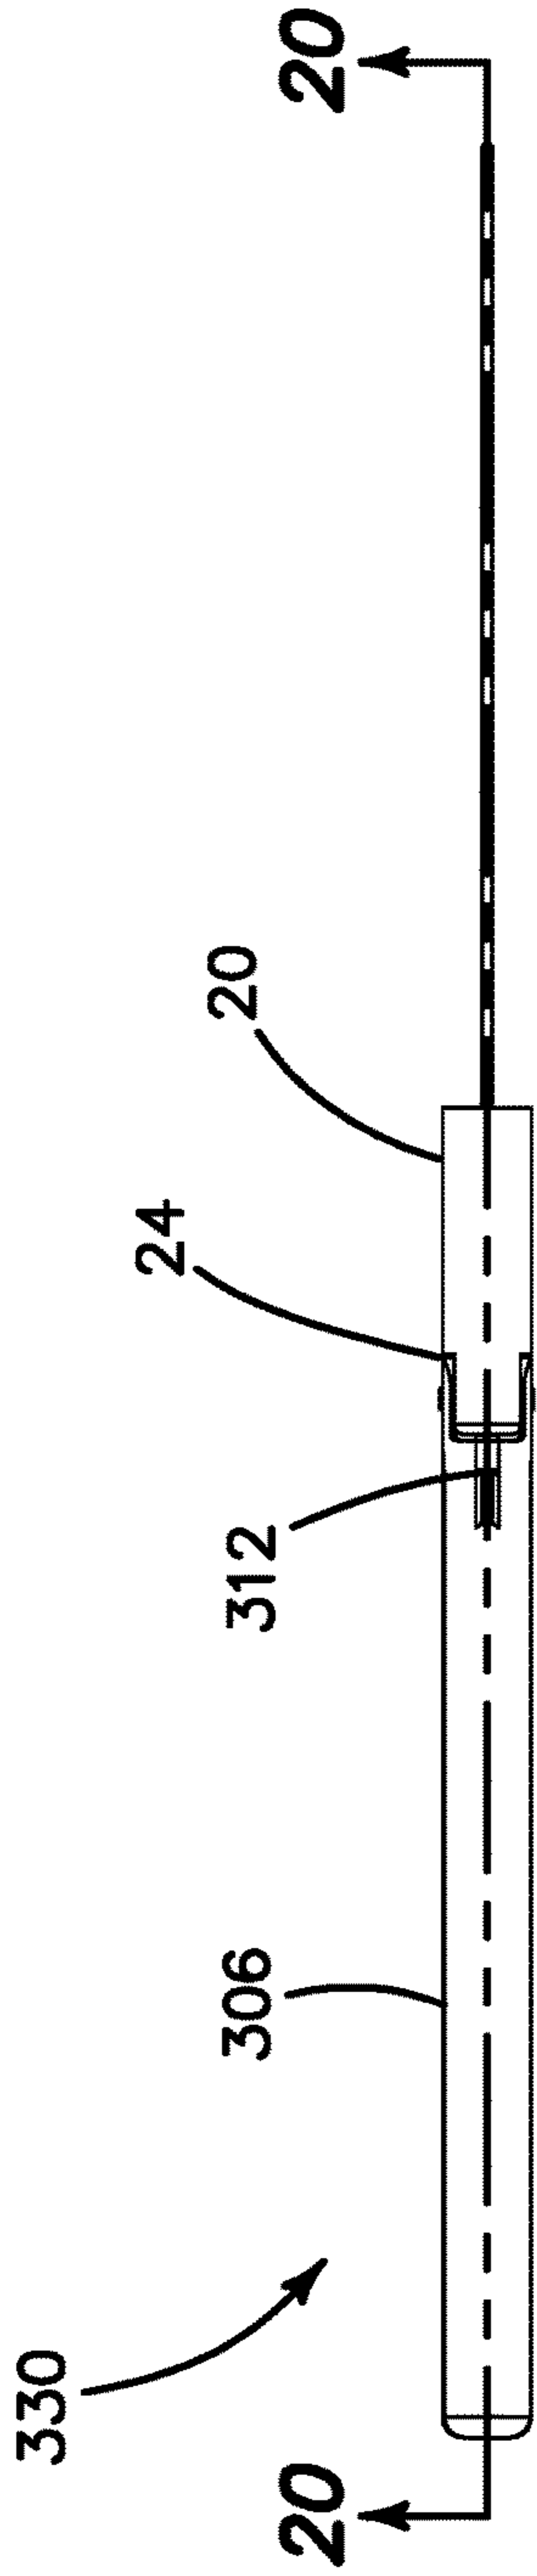


FIG. 18

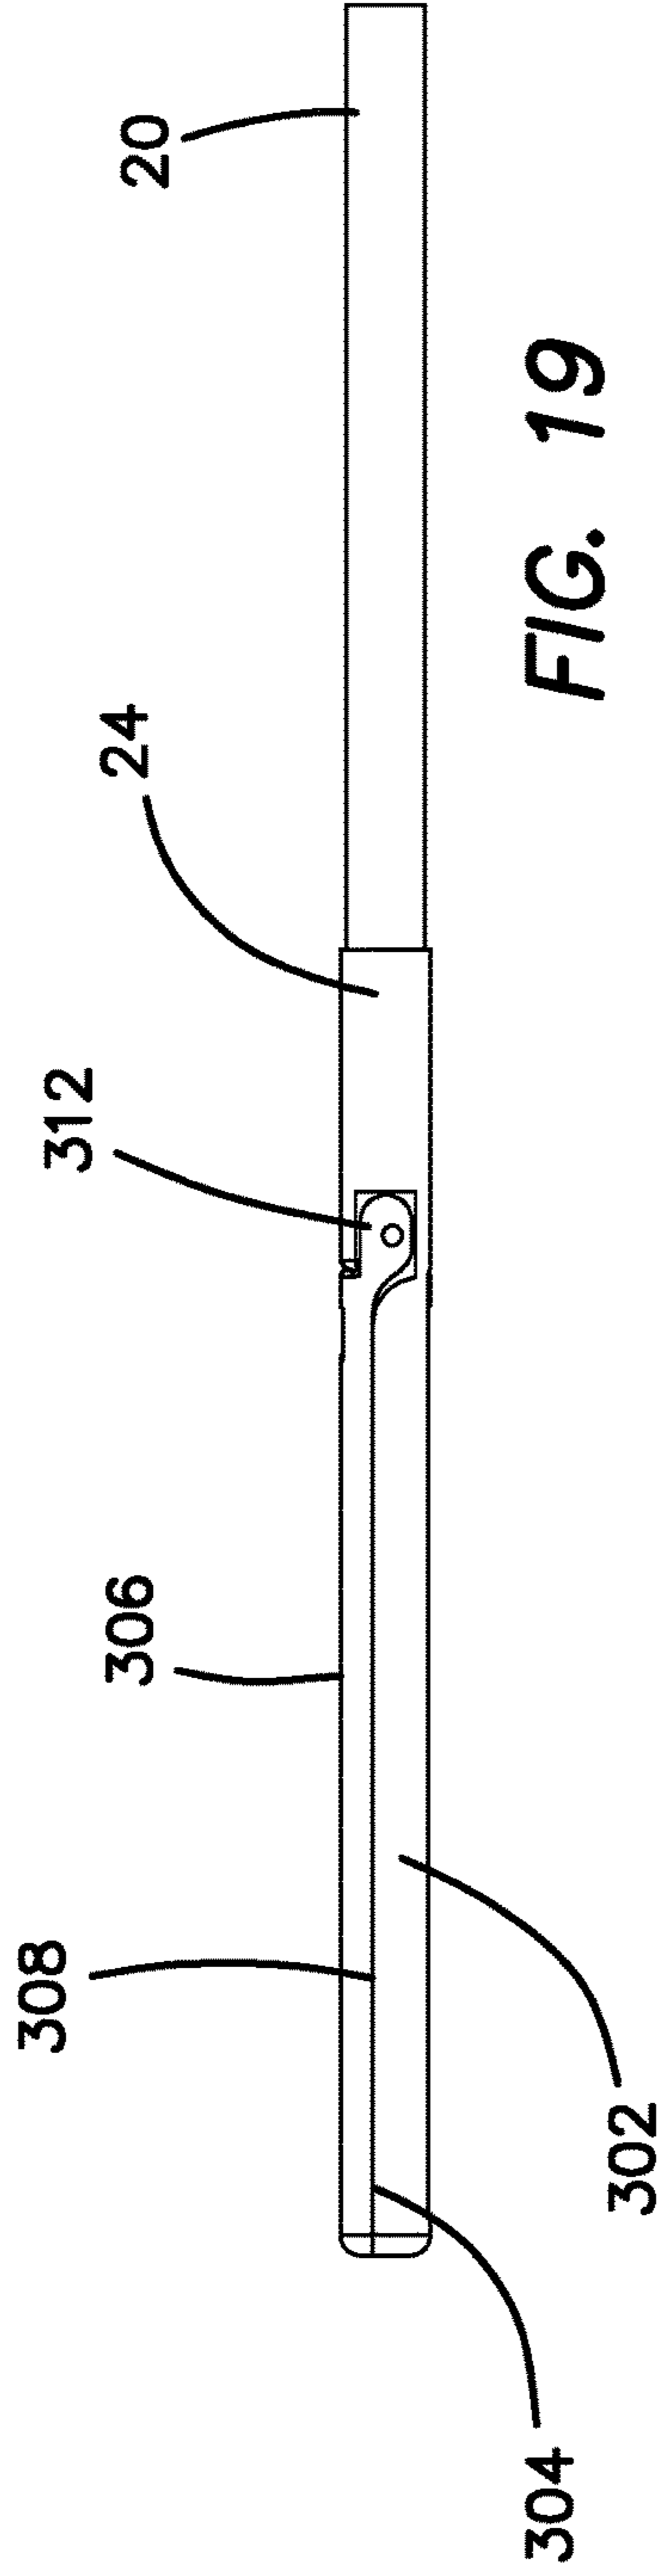


FIG. 19

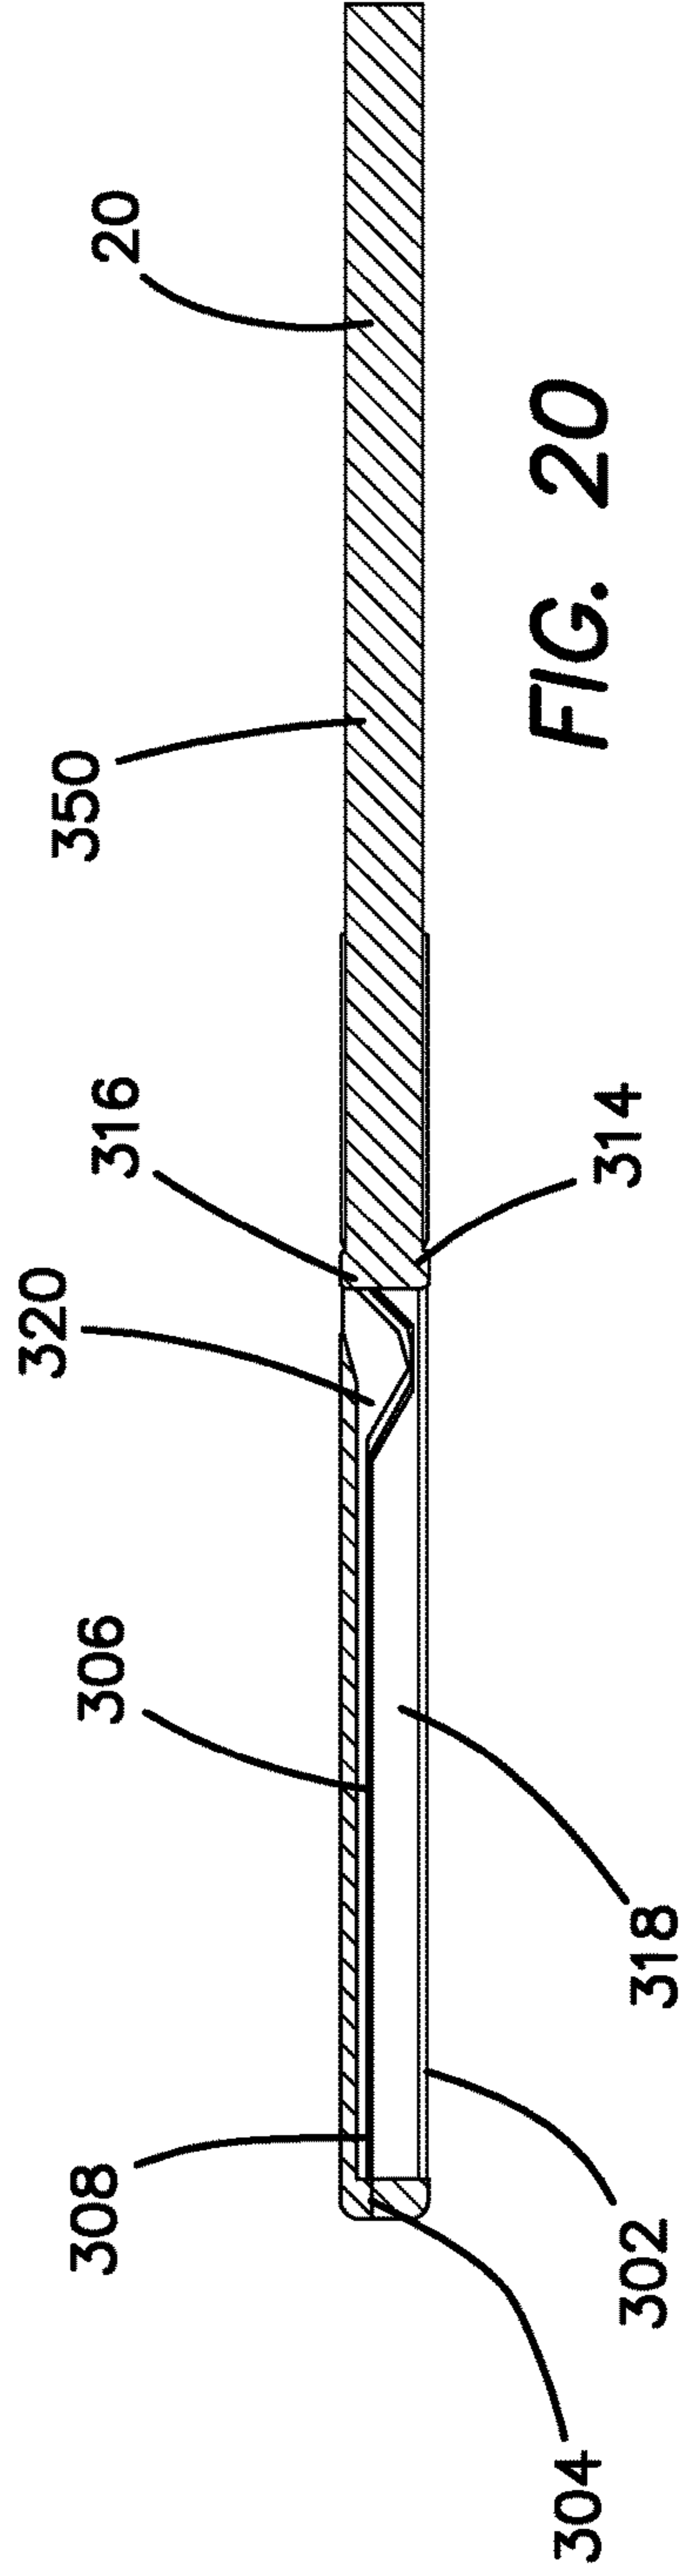
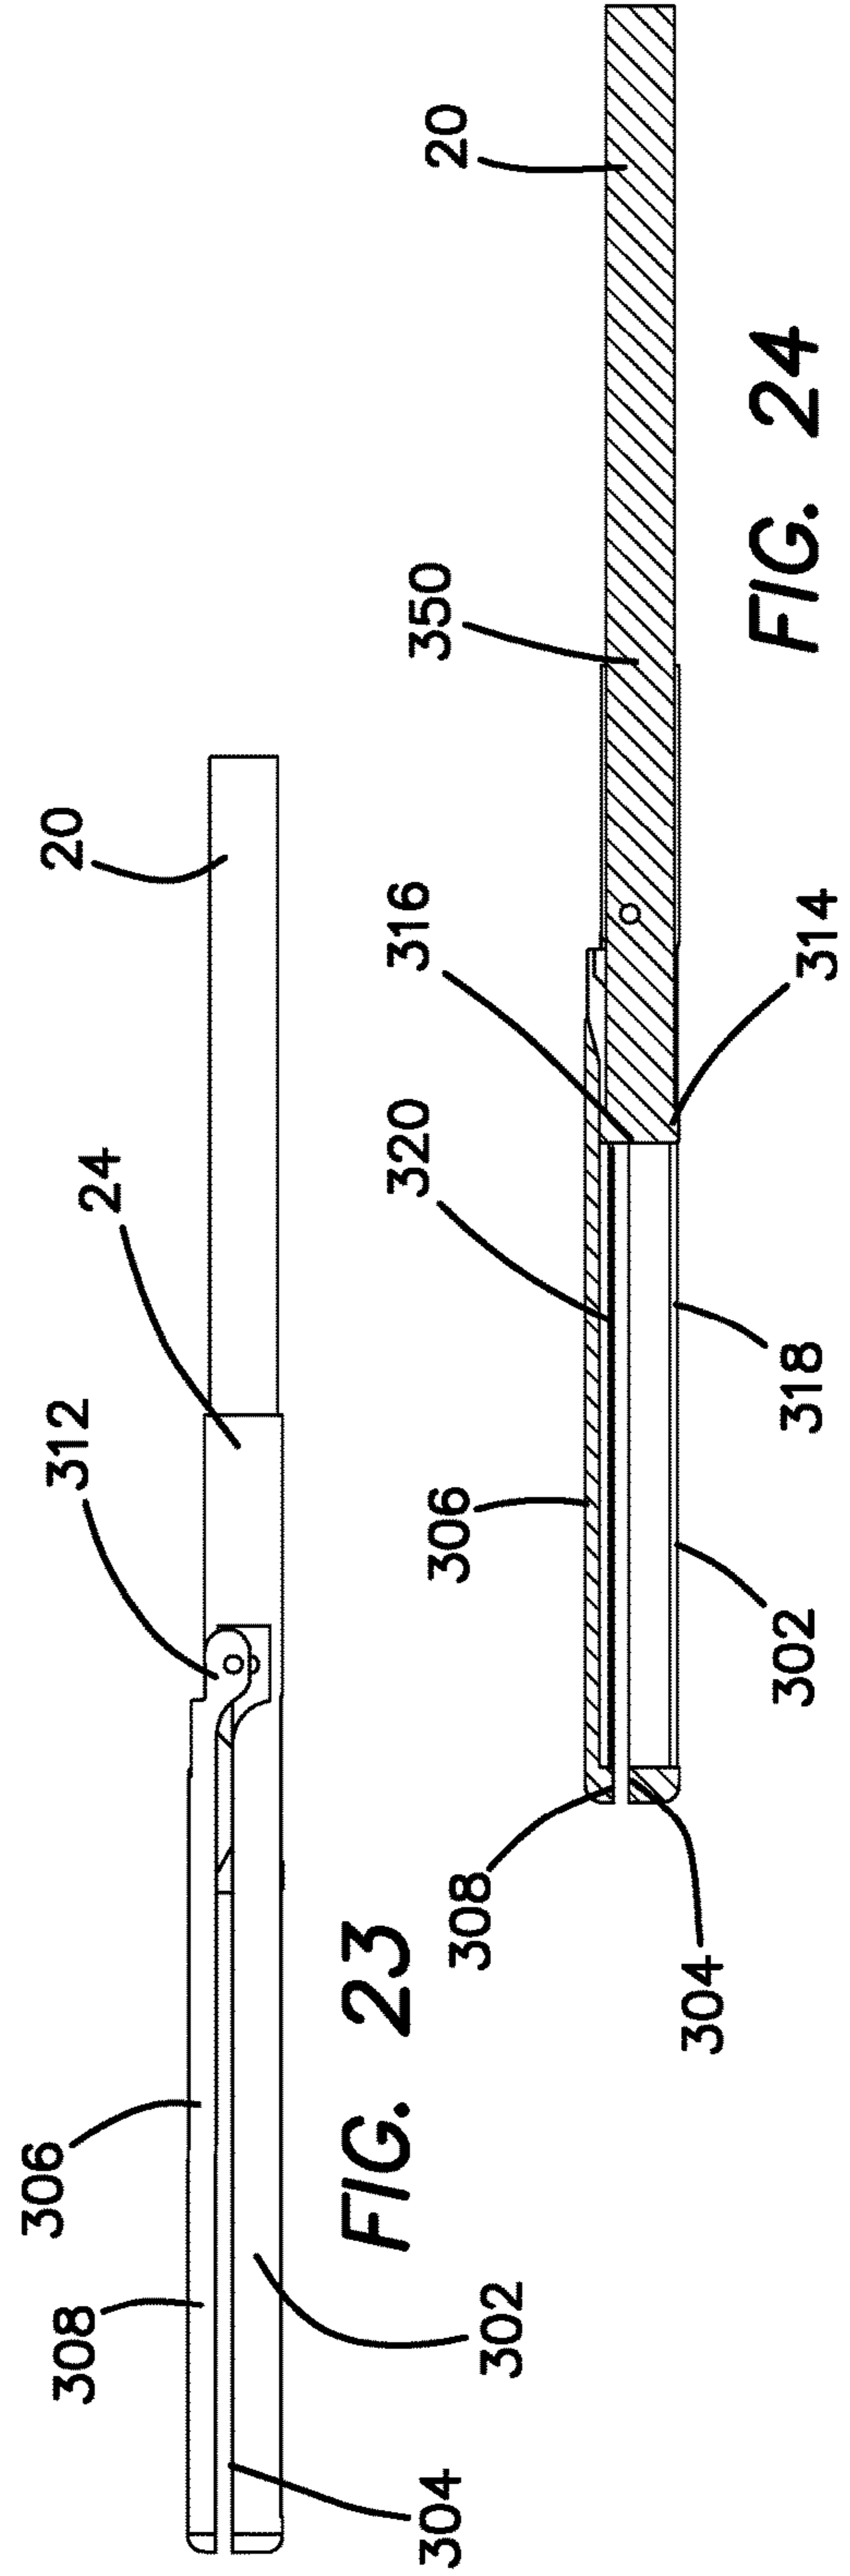
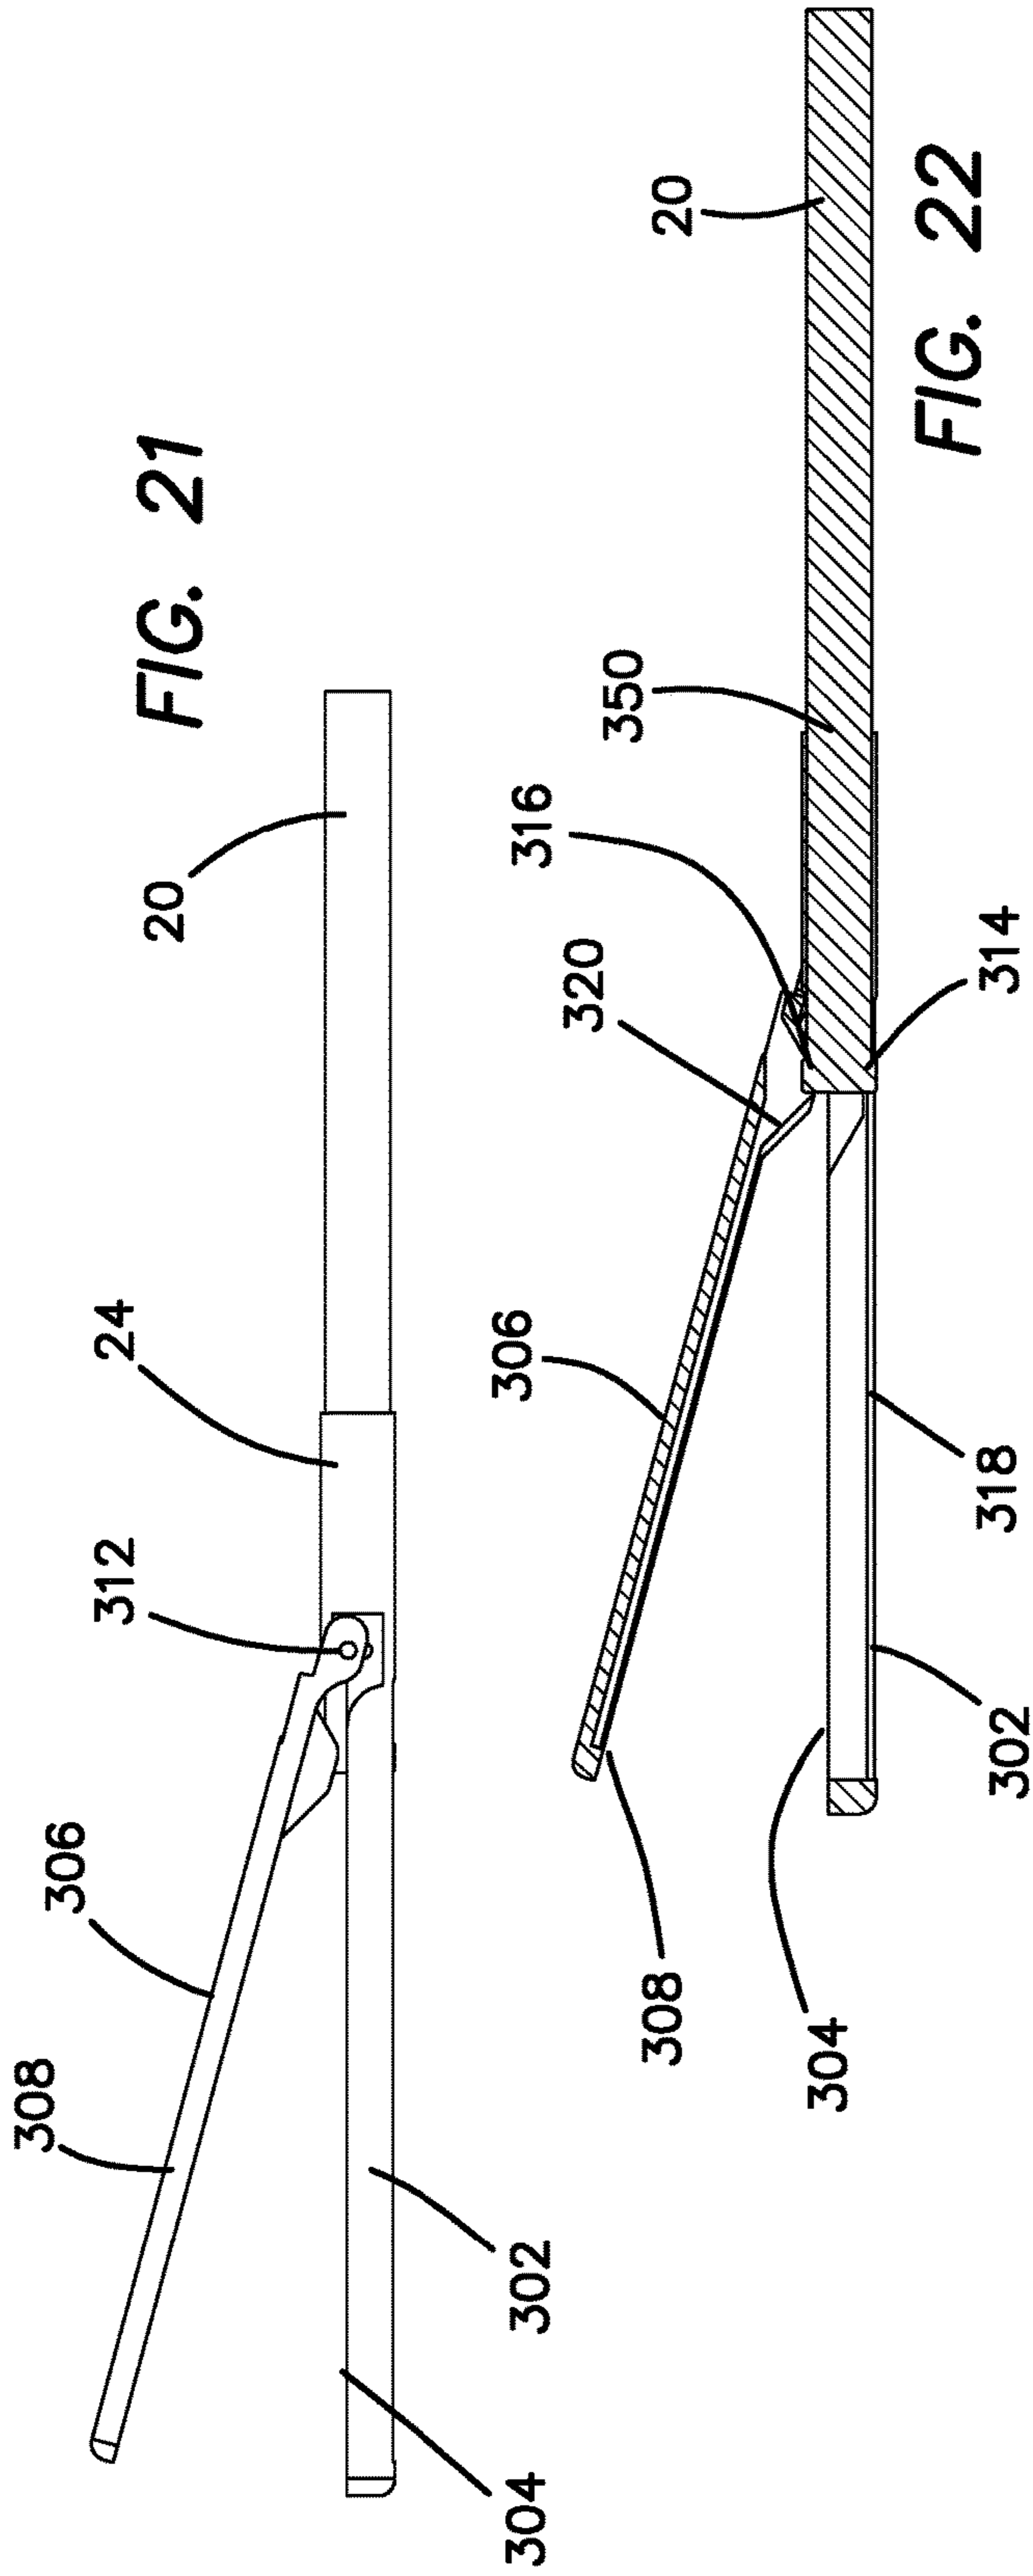


FIG. 20



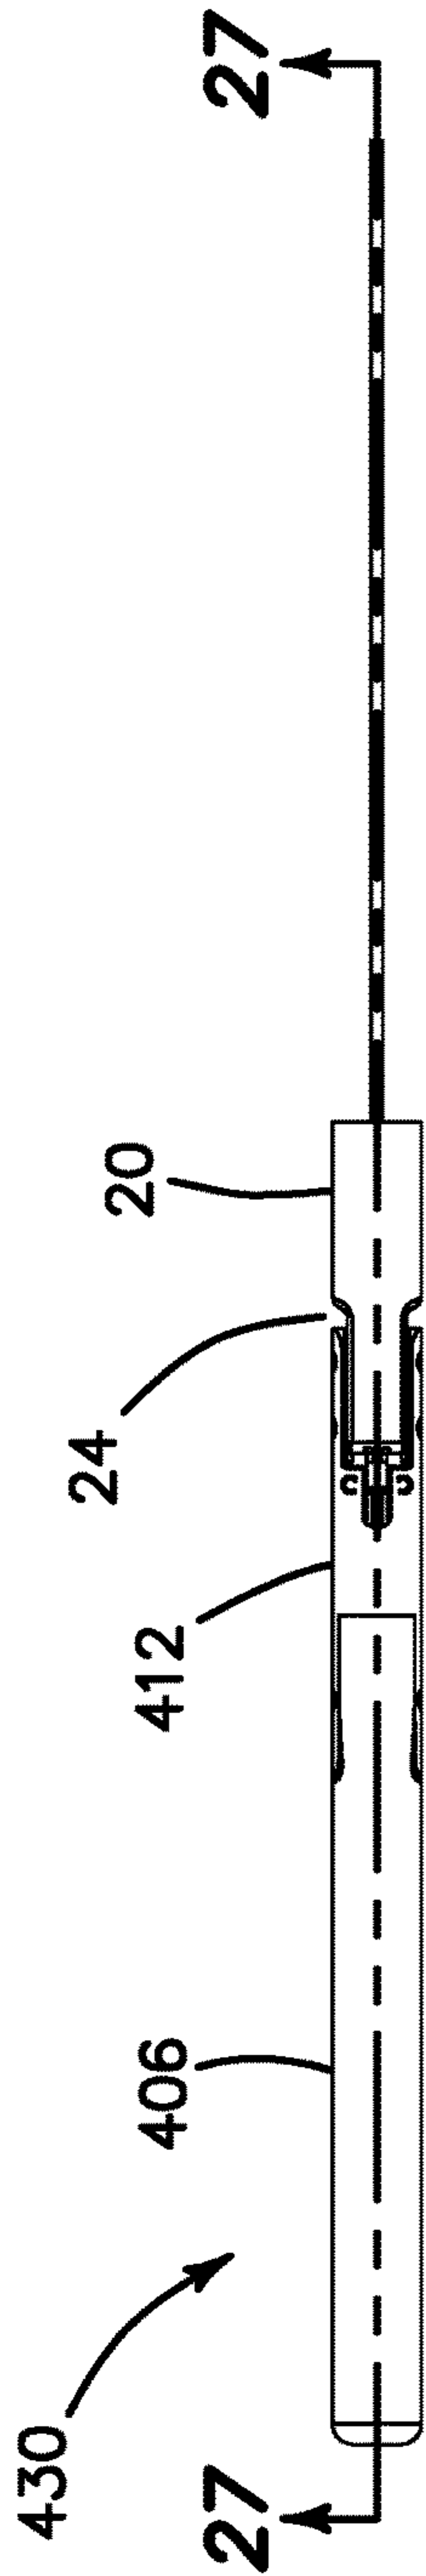


FIG. 25

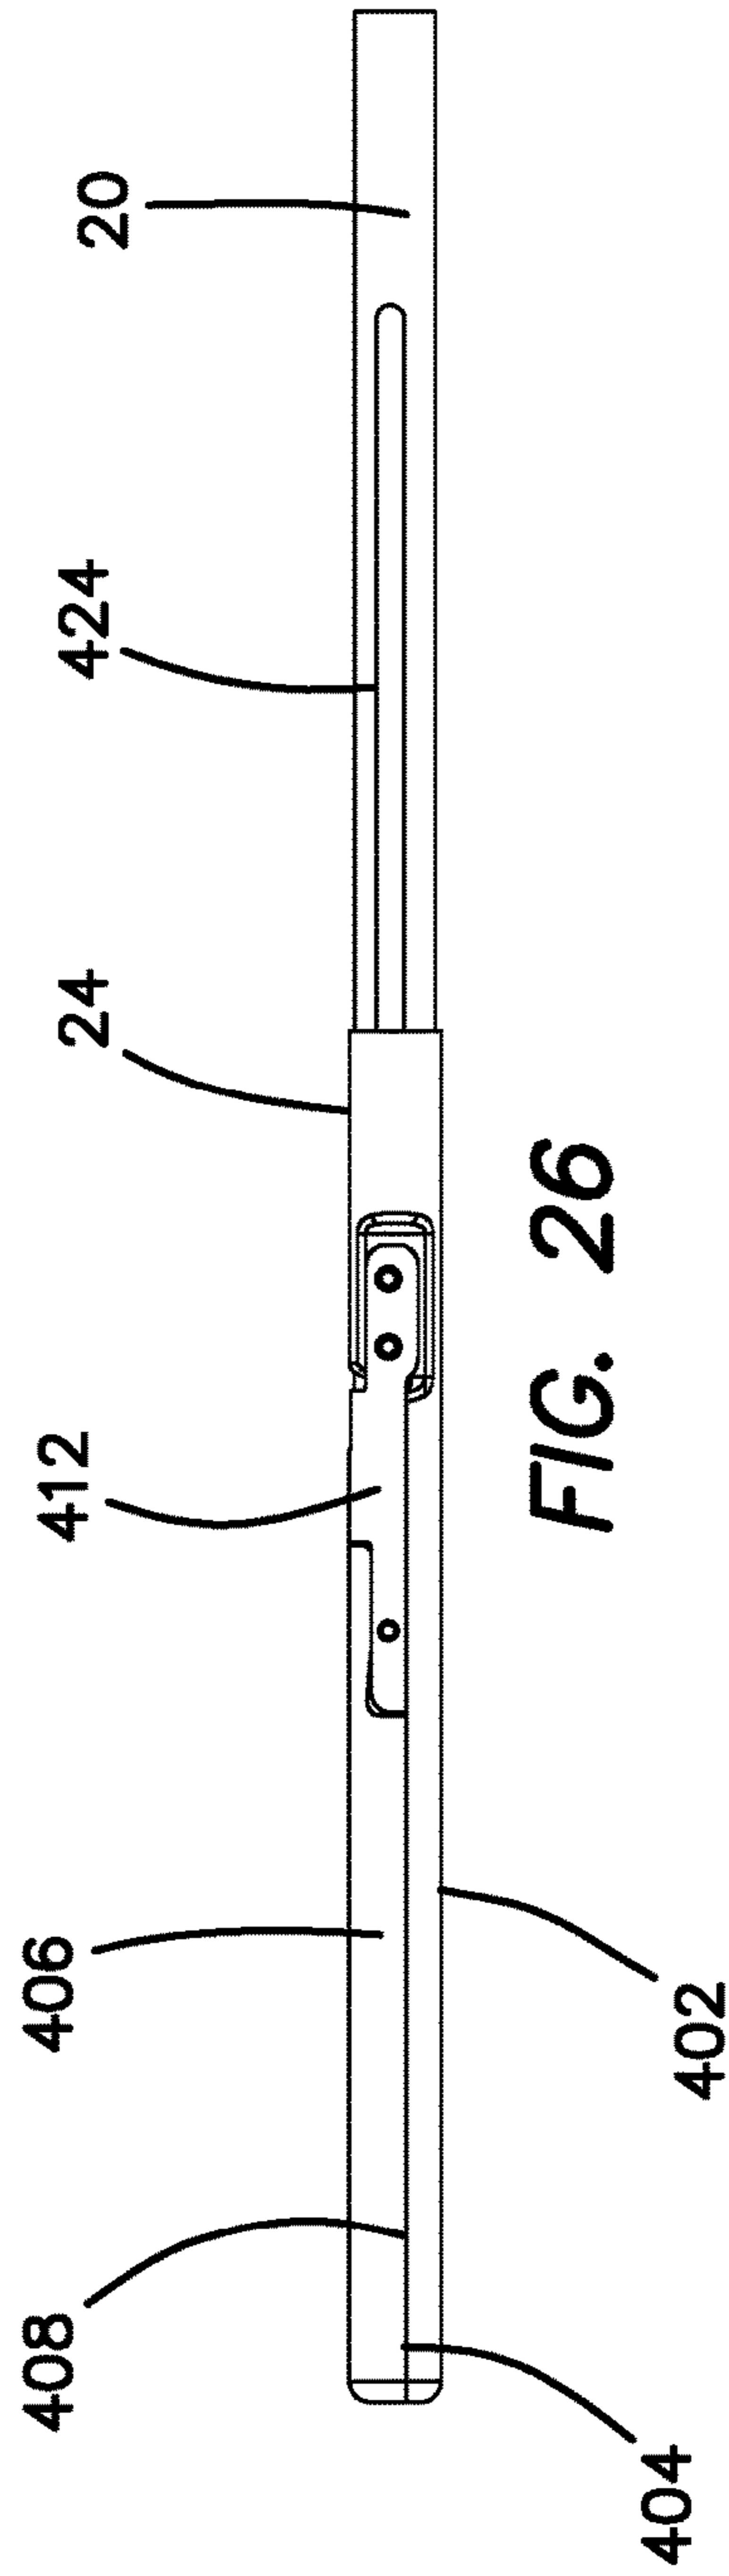


FIG. 26

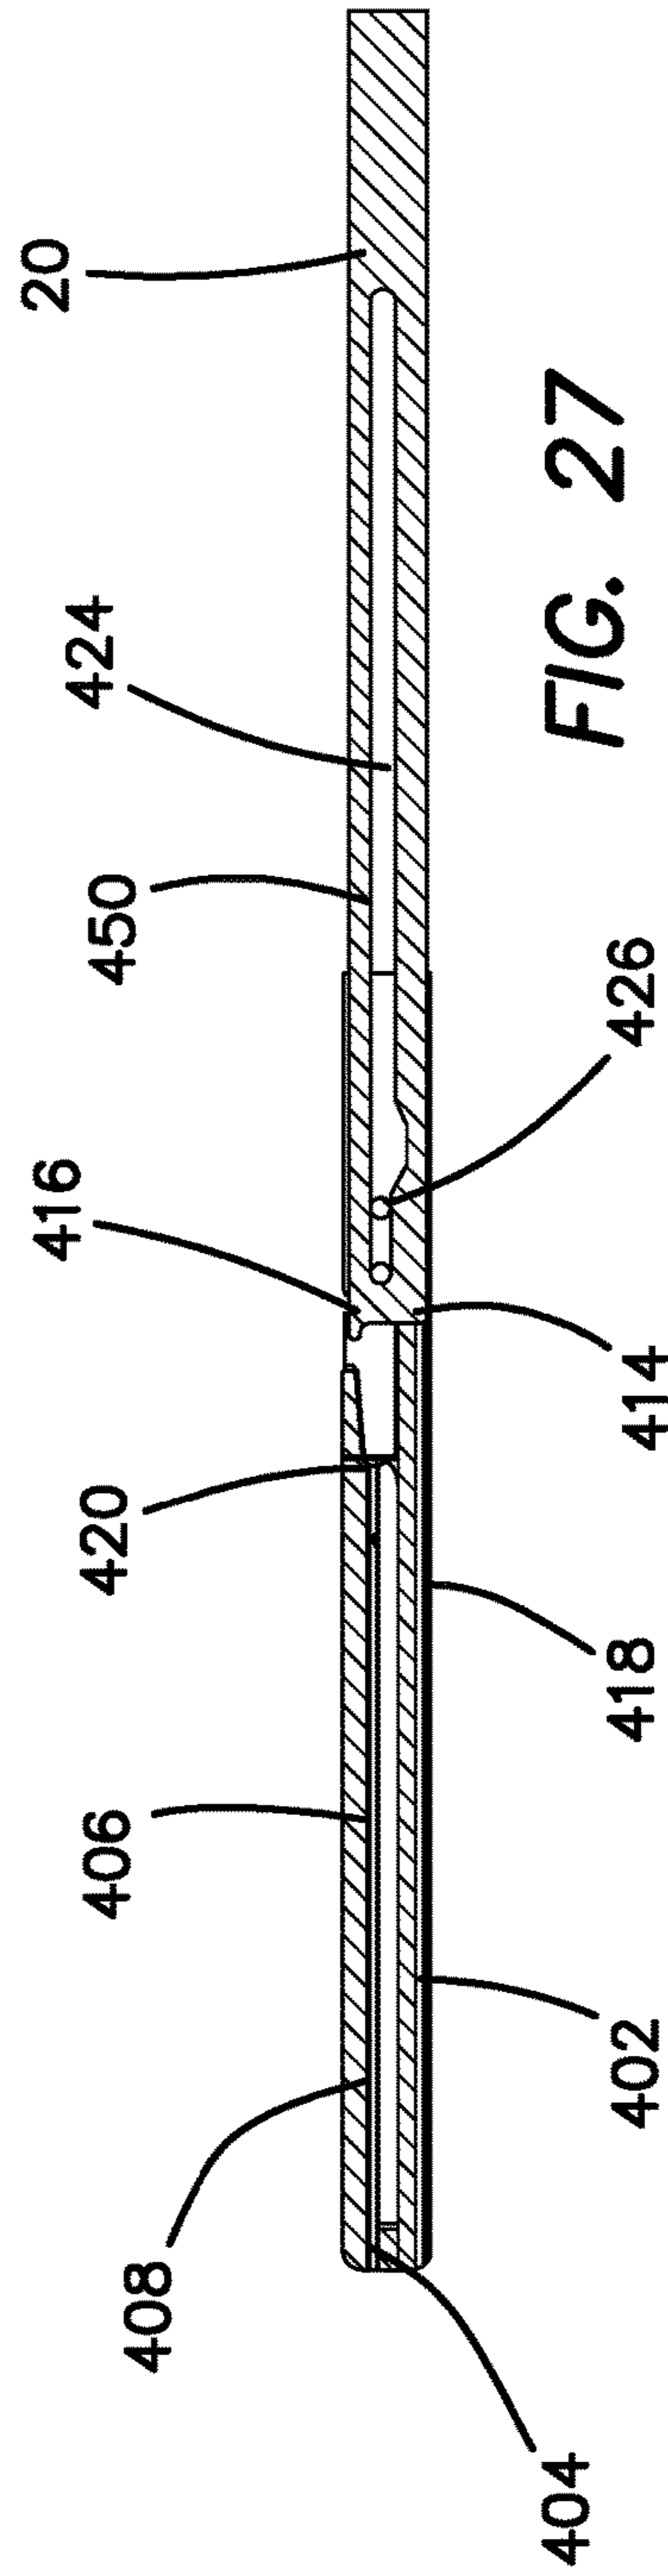


FIG. 27

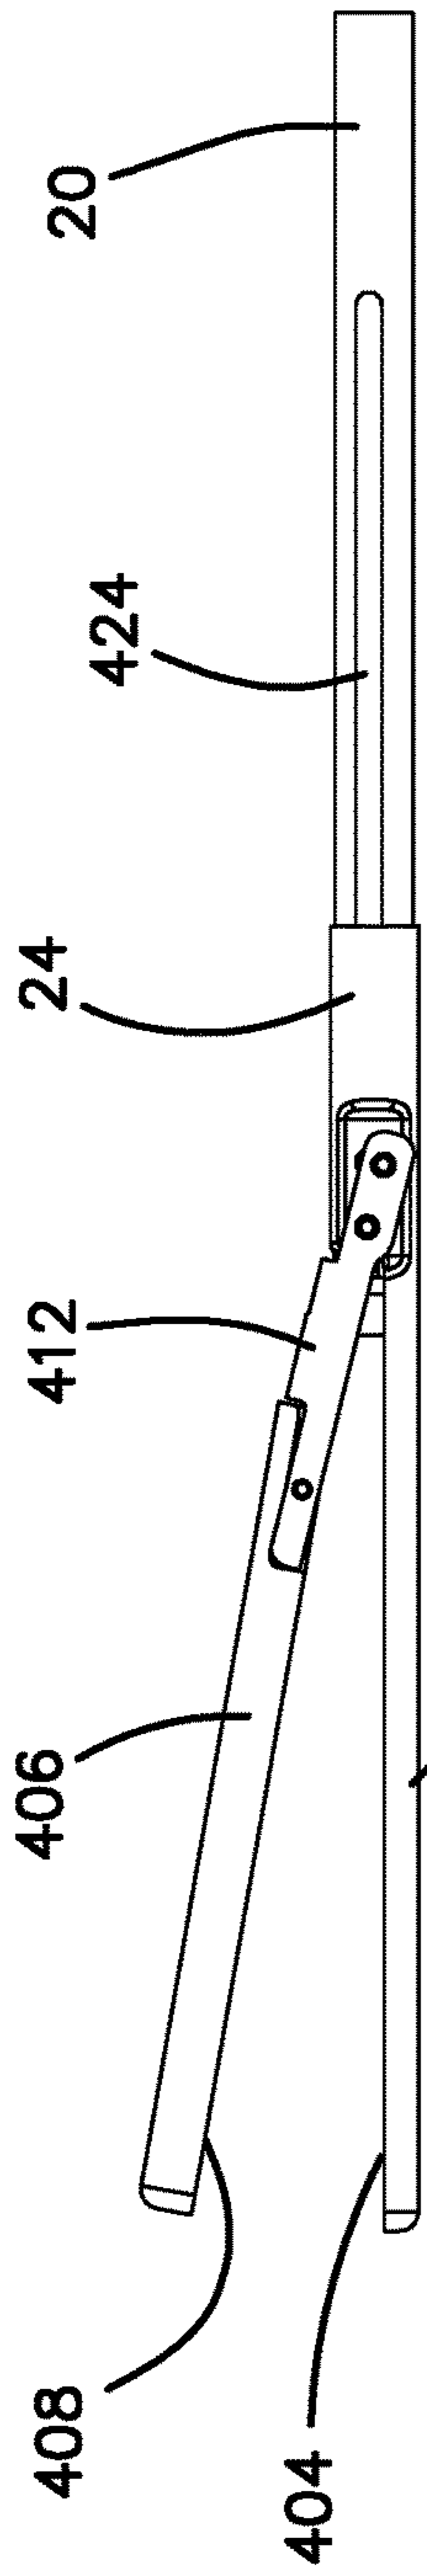


FIG. 28

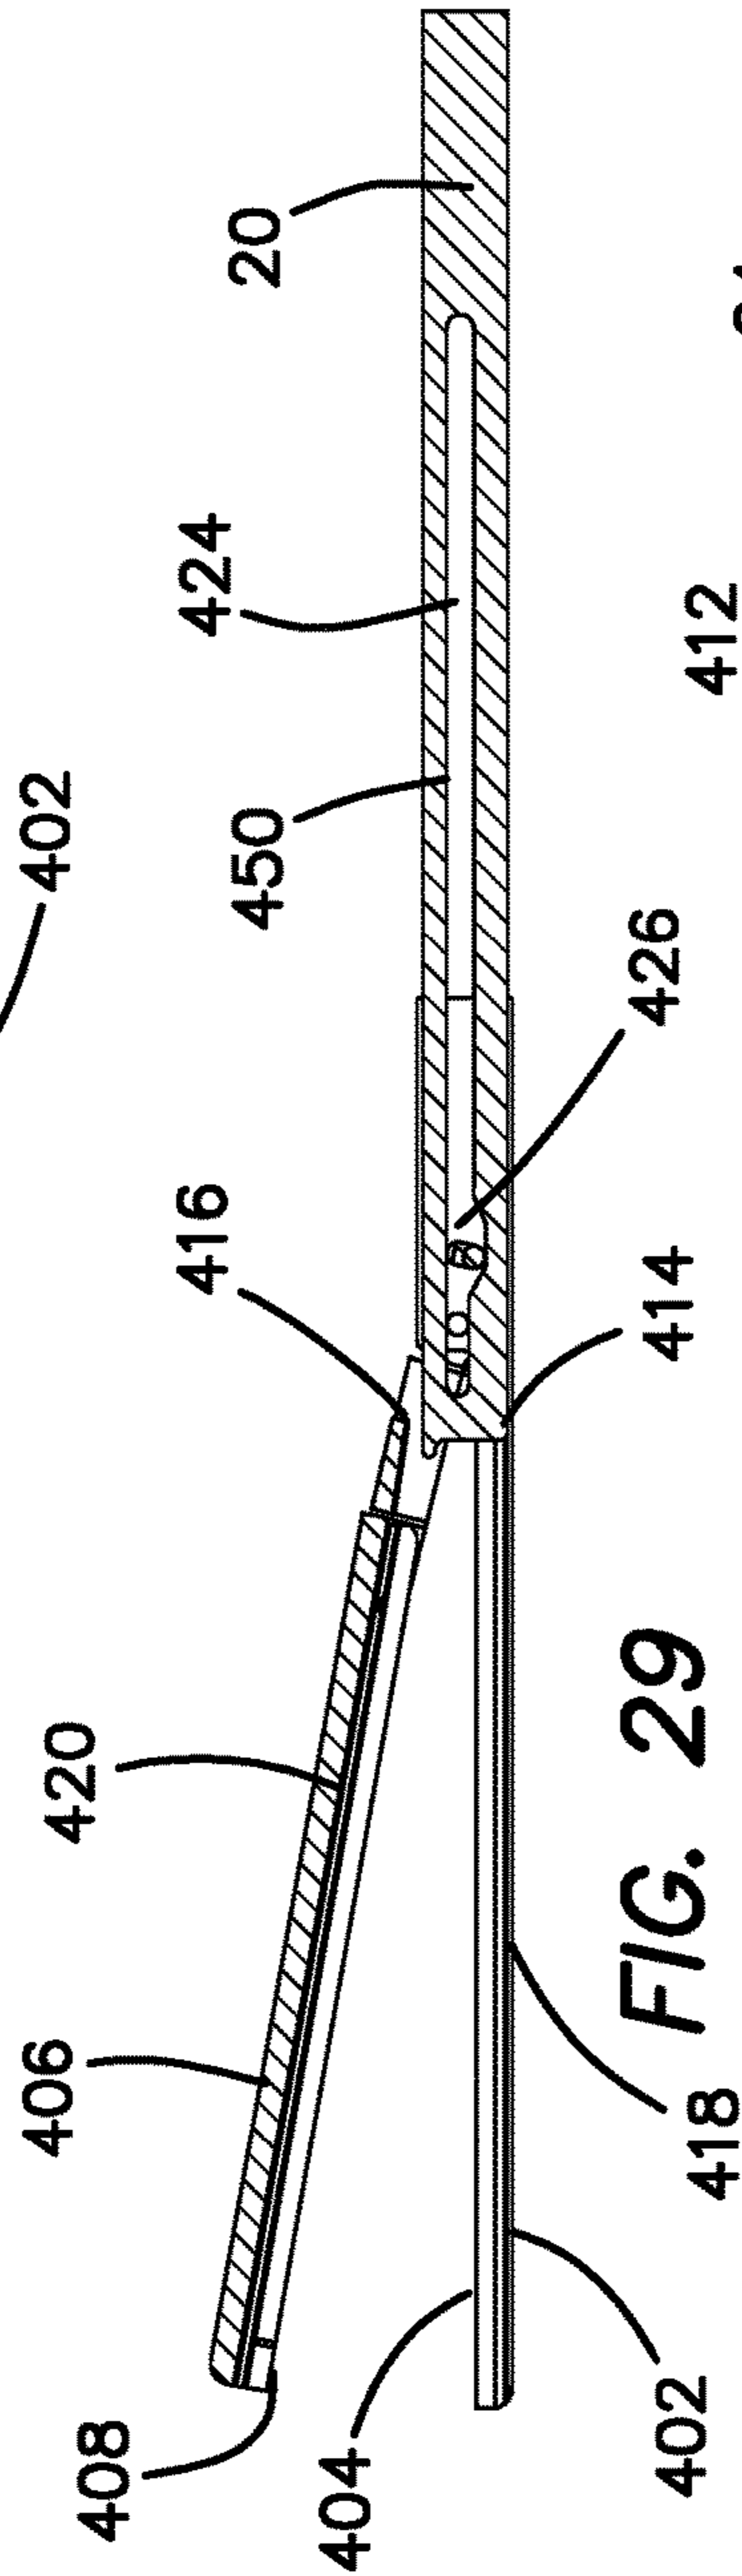


FIG. 29

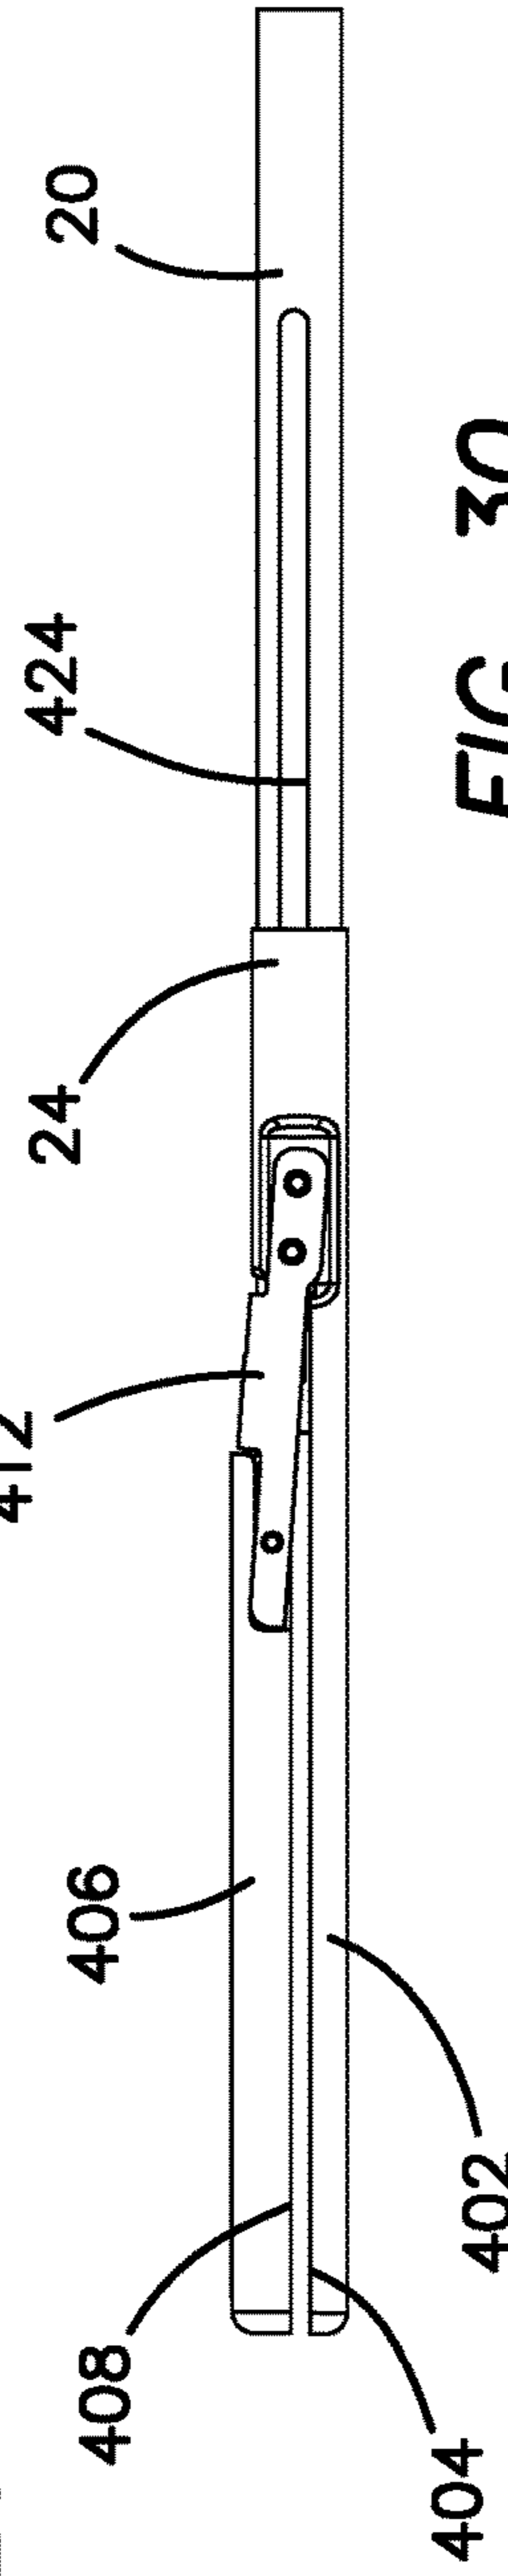


FIG. 30






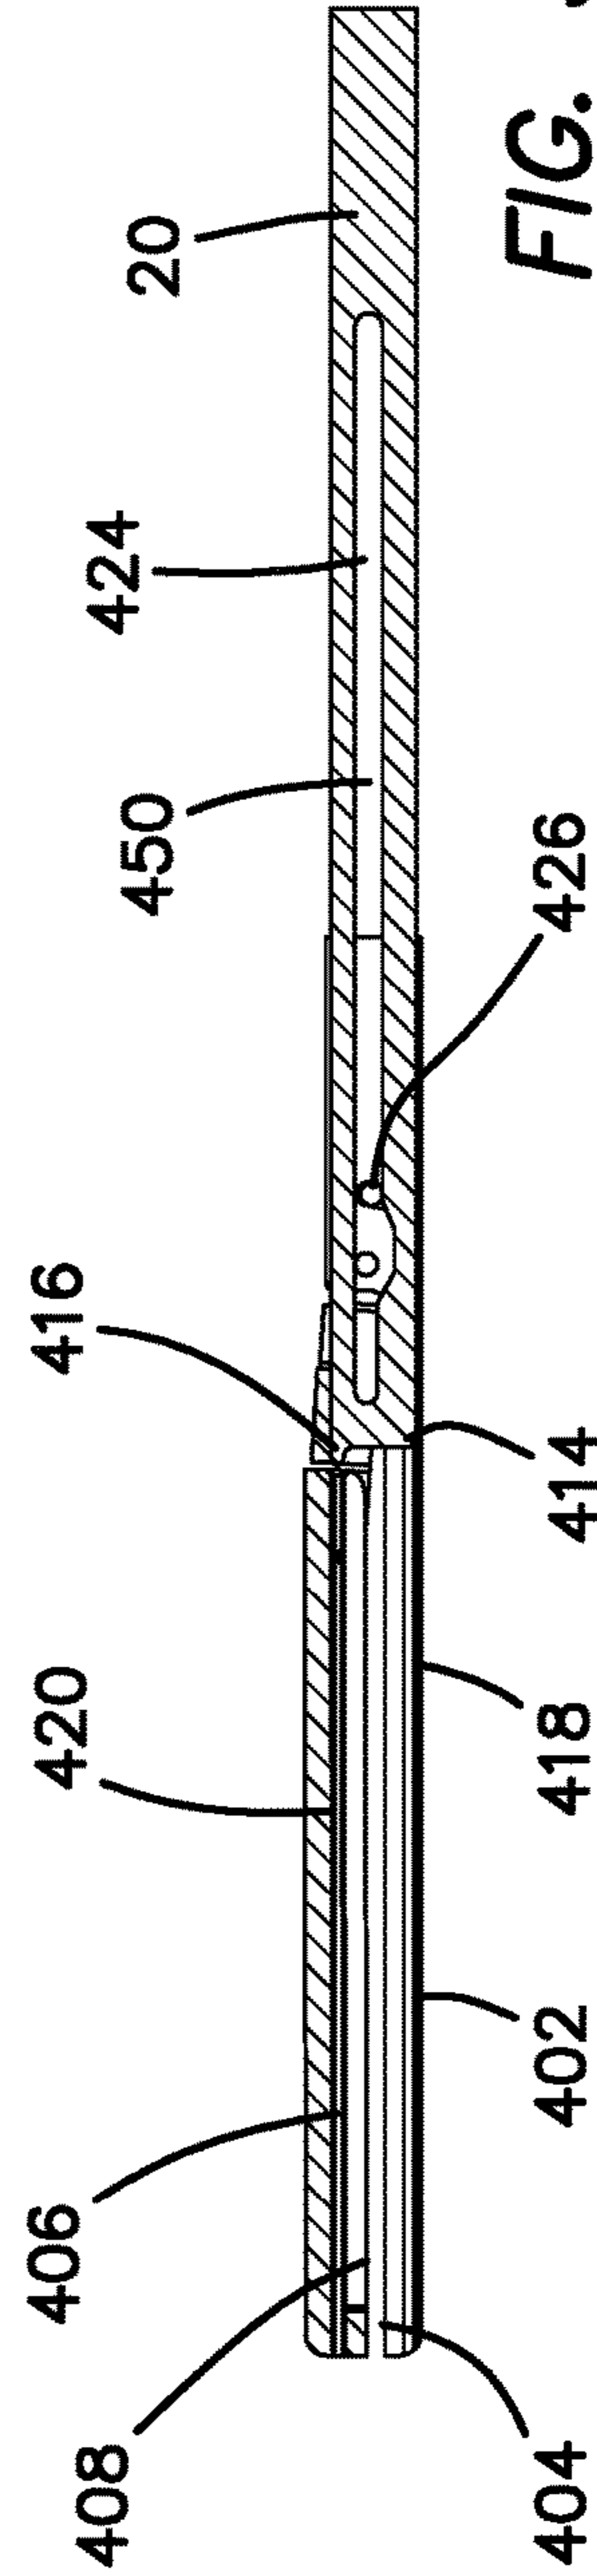


FIG. 31

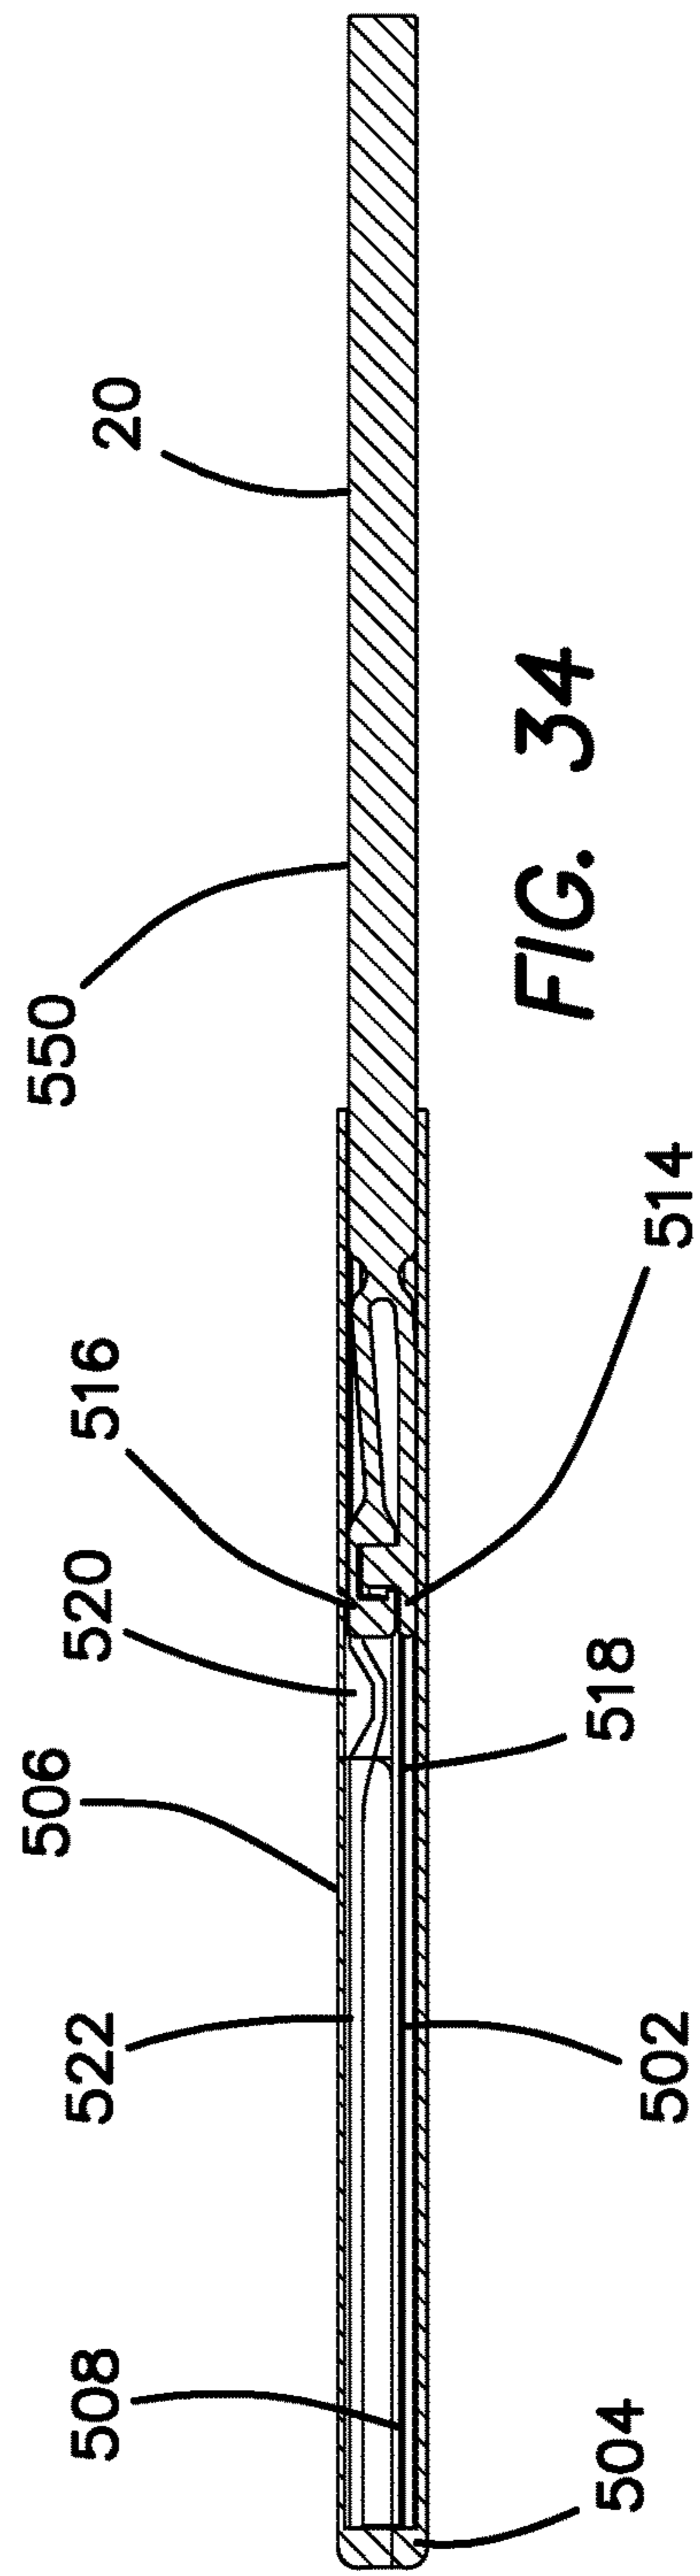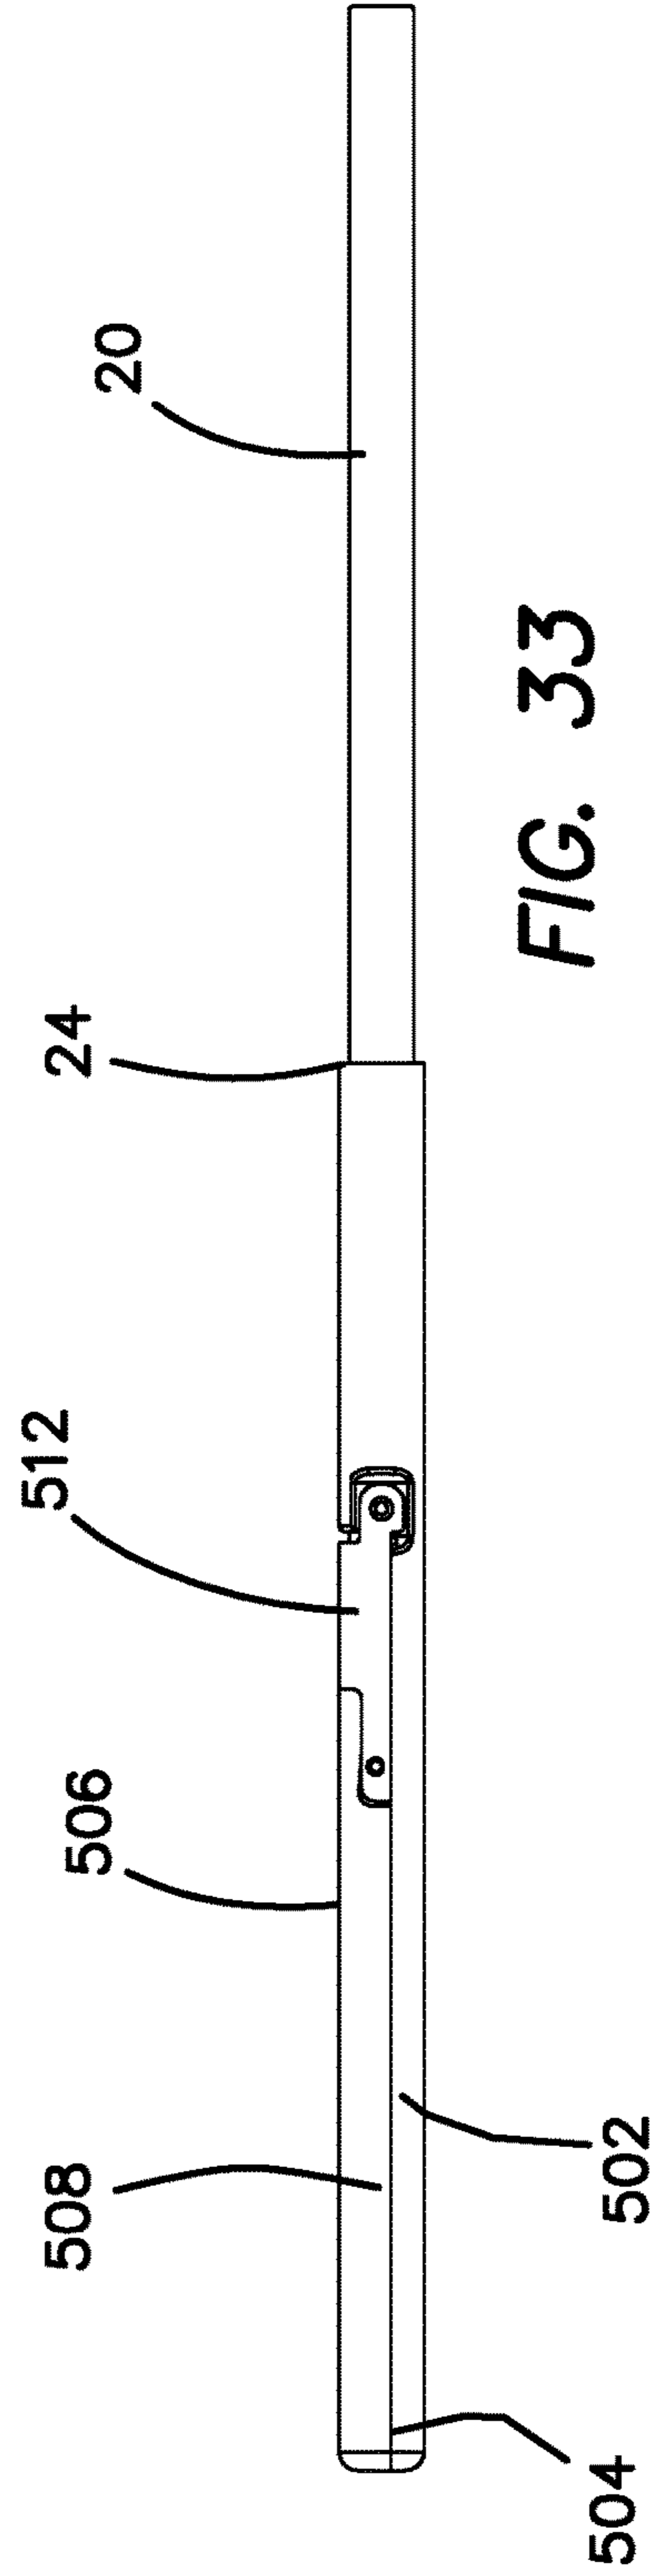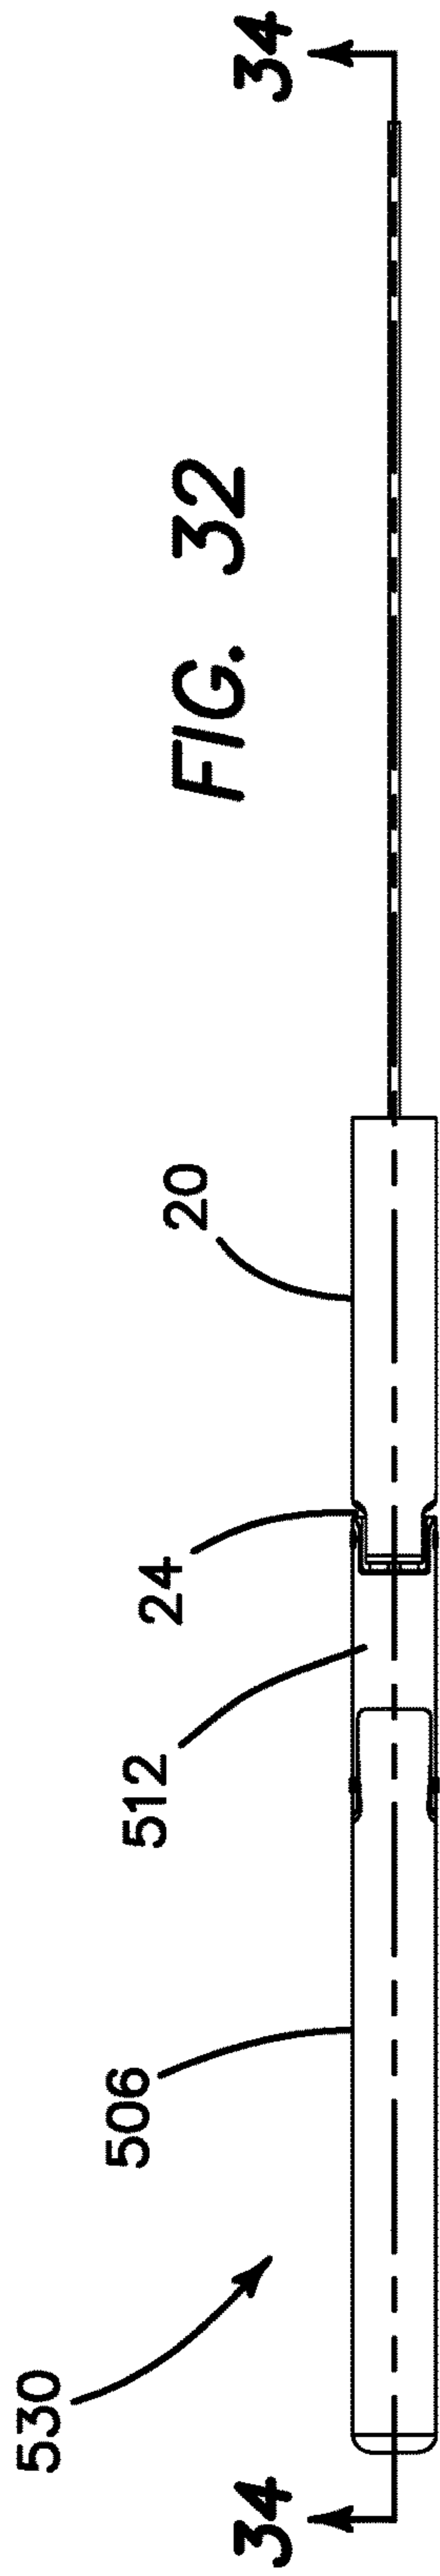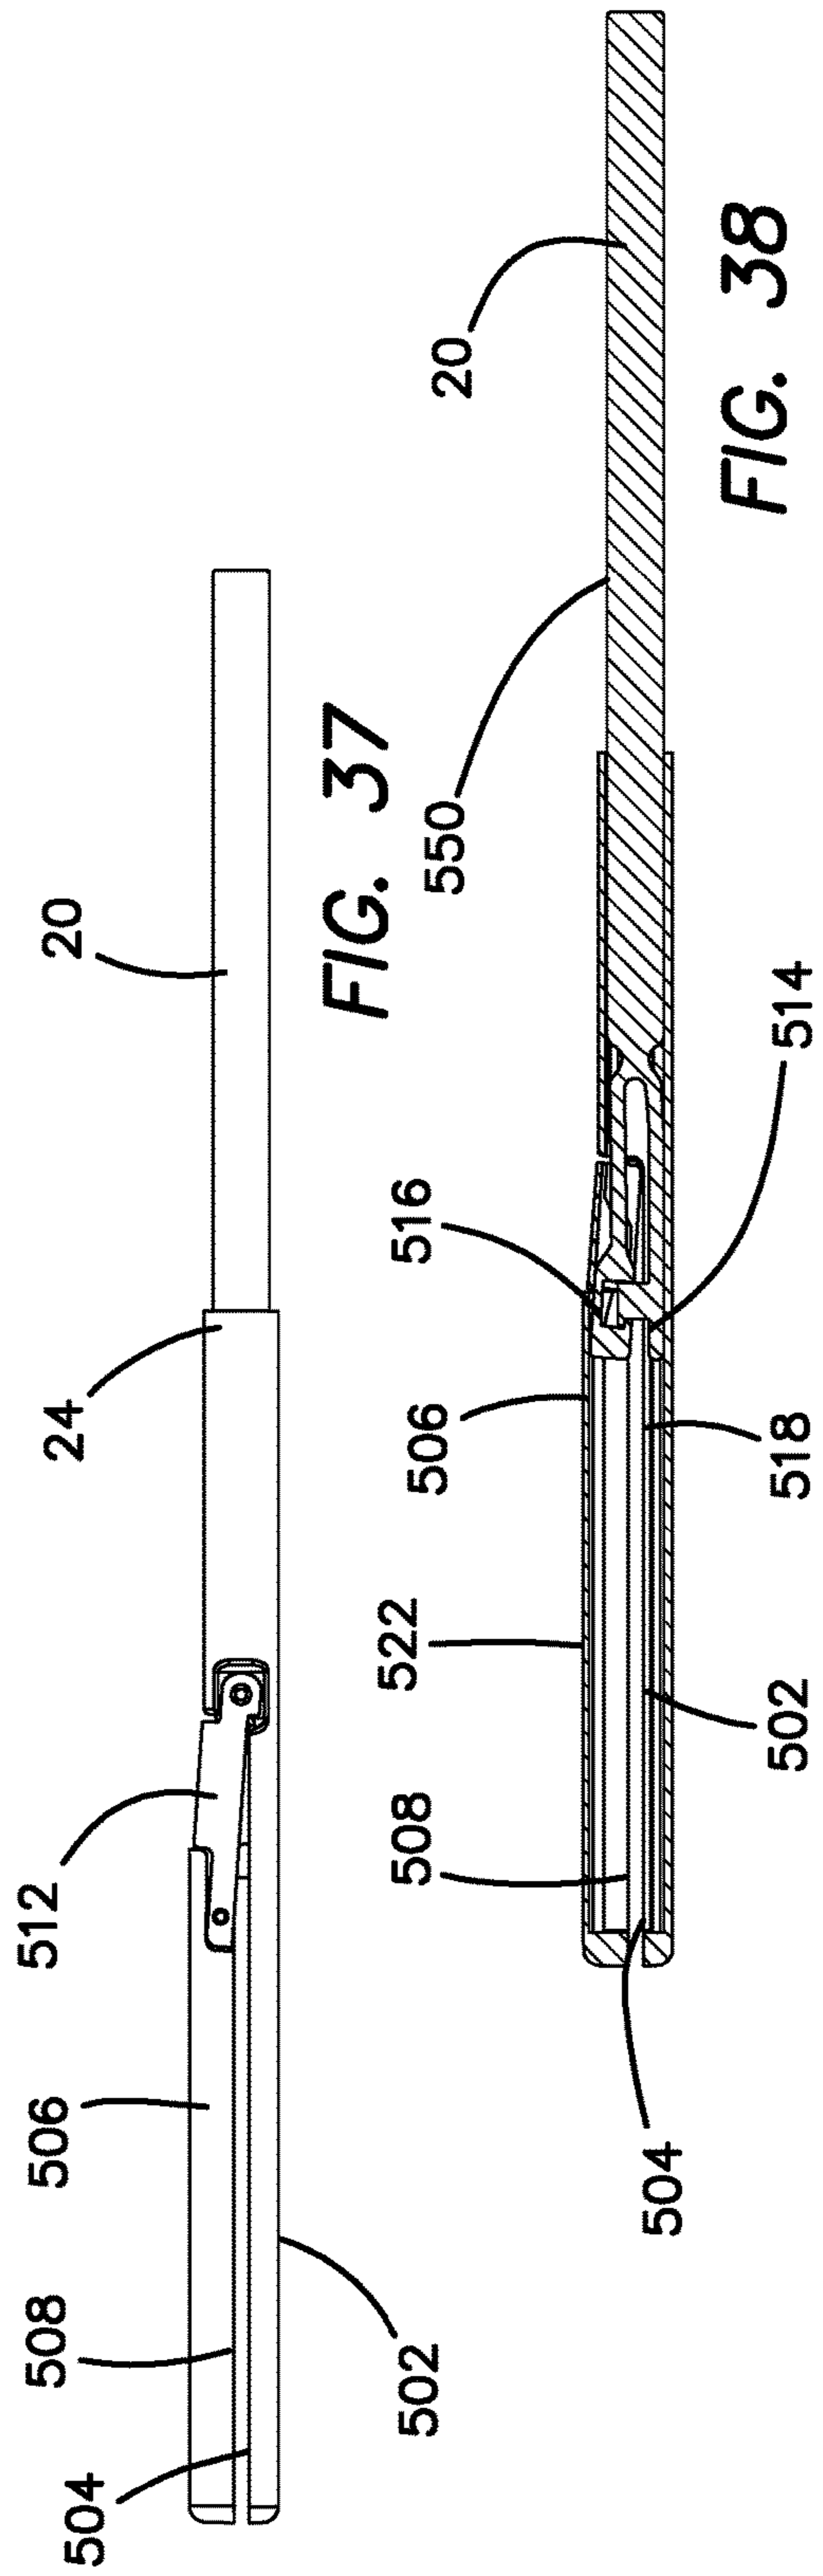

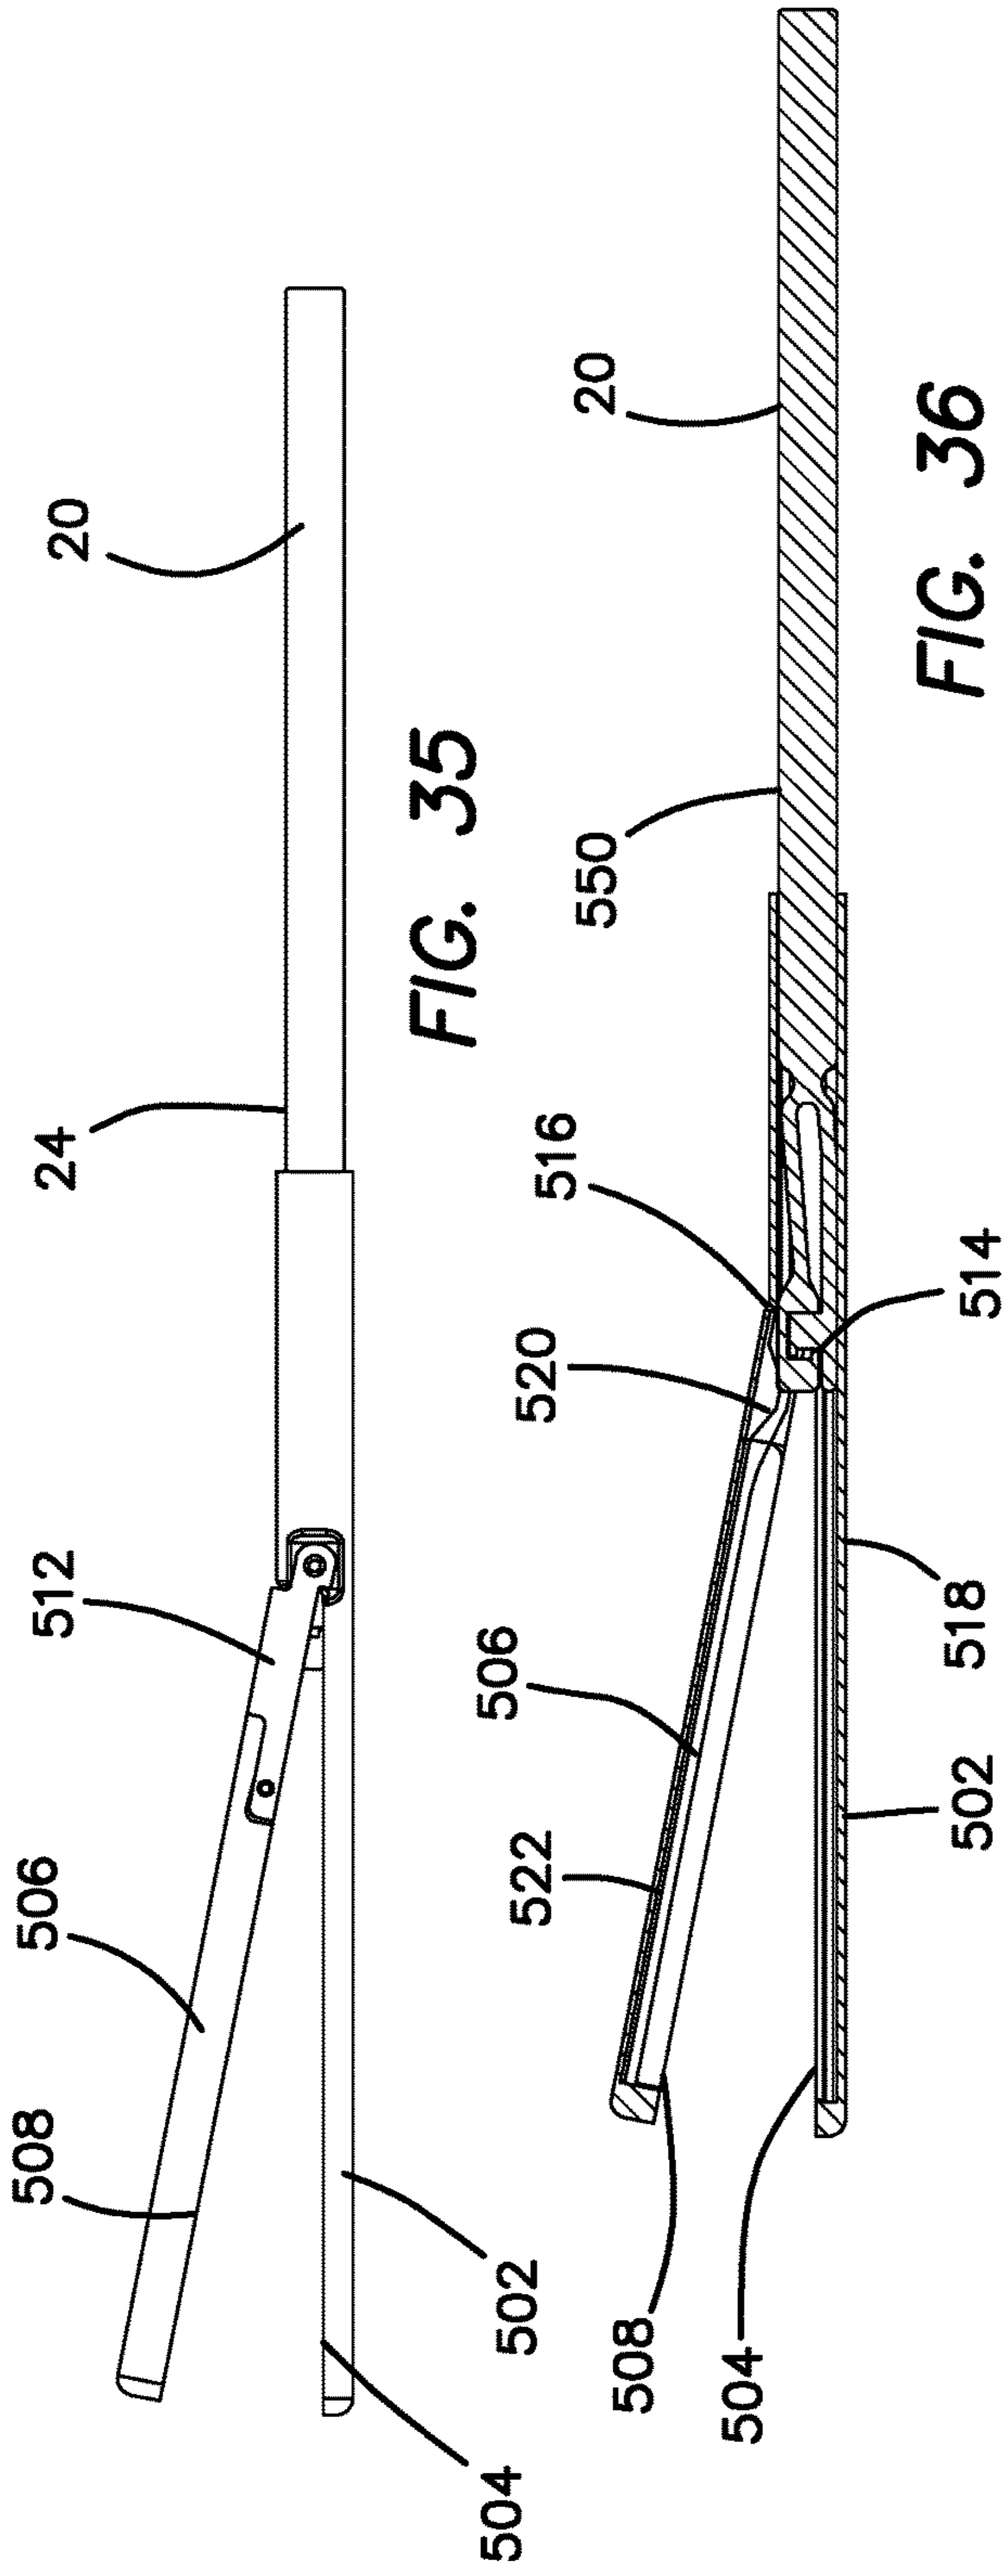

## SURGICAL STAPLER WITH EXPANDABLE JAW

### CROSS REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of U.S. Provisional Patent Application Ser. No. 61/793,065, entitled "SURGICAL STAPLER WITH EXPANDABLE JAW," filed on Mar. 15, 2013. The entirety of this prior application is hereby incorporated herein by reference.

### BACKGROUND OF THE INVENTION

#### Field of the Invention

The present application relates generally to surgical occlusion instruments and, more particularly, to surgical staplers.

#### Description of the Related Art

Surgical staplers are used to approximate or clamp tissue and to staple the clamped tissue together. As such, surgical staplers have mechanisms to ensure that tissue is properly positioned and captured and to drive staples through the tissue. As a result, this has produced, for example, multiple triggers and handles in conjunction with complex mechanisms to provide proper stapling of the clamped tissue. With these complex mechanisms, surgical staplers can have increased manufacturing burdens, as well as potential sources for device failure and confusion for the user. Thus, reliable stapling of clamped tissue without complex mechanisms is desired.

### SUMMARY OF THE INVENTION

In certain embodiments, a surgical stapler is provided herein. The surgical stapler comprises an elongate shaft, a handle assembly, an actuation mechanism, and a jaw assembly. The elongate shaft has a proximal end and a distal end and defines a longitudinal axis between the proximal end and the distal end. The handle assembly is disposed at the proximal end of the elongate shaft. The actuation mechanism is actuatable by the handle assembly. The actuation mechanism comprises an actuation beam extending through at least a portion of the elongate shaft. The jaw assembly is disposed at the distal end of the elongate shaft. The jaw assembly comprises a first jaw, a second jaw, and a plurality of staples positioned in the first jaw. The first jaw defines a first clamping surface. The second jaw defines a second clamping surface. The jaw assembly is actuatable by longitudinal movement of the actuation beam between a closed position in which the first clamping surface contacts the second clamping surface, an open position in which the second clamping surface extends at an angle transverse to the first clamping surface, and a stapling position in which the first clamping surface extends parallel to the second clamping surface and is spaced apart from the second clamping surface.

In certain embodiments, a surgical stapler is provided herein. The surgical stapler comprises an elongate shaft, a handle assembly, an actuation mechanism, and a jaw assembly. The elongate shaft has a proximal end and a distal end and defines a longitudinal axis between the proximal end and the distal end. The handle assembly is disposed at the proximal end of the elongate shaft. The actuation mechanism is actuatable by the handle assembly. The actuation mechanism comprises an actuation member extending through at least a portion of the elongate shaft. The actuation

member comprises a first guide and a second guide thereon. The jaw assembly is disposed at the distal end of the elongate shaft. The jaw assembly comprises a first jaw, a link, and a second jaw. The first jaw extends distally from the distal end of the elongate shaft. The first jaw comprises a first guide slot extending longitudinally therein. The link has a proximal end and a distal end. The link comprises a second guide slot having a ramped opening profile formed therein. The proximal end of the link is pivotably coupled to the distal end of the elongate shaft. The second jaw extends distally from the distal end of the link. The second jaw is pivotably coupled to the distal end of the link. The second jaw comprises a third guide slot extending longitudinally therein. A plurality of staples is disposed in the first jaw. The first guide is slideable in the first guide slot and the second guide is slideable in the second guide slot and the third guide slot. Translation of the second guide distally over the ramped opening profile of the second guide slot pivots the link away from the first jaw to define an open position of the jaw assembly.

In certain embodiments, a surgical stapler is provided herein. The surgical stapler comprises an elongate shaft, a handle assembly, an actuation mechanism, and a jaw assembly. The elongate shaft has a proximal end and a distal end and defines a longitudinal axis between the proximal end and the distal end. The handle assembly is disposed at the proximal end of the elongate shaft. The actuation mechanism is actuatable by the handle assembly. The actuation mechanism comprises an actuation member extending through at least a portion of the elongate shaft. The actuation member comprises a first guide and a second guide thereon. The jaw assembly is disposed at the distal end of the elongate shaft. The jaw assembly comprises a first jaw, a second jaw, and a plurality of staples. The first jaw extends distally from the distal end of the elongate shaft. The first jaw comprises a first guide slot extending longitudinally therein and a first clamping surface. The second jaw comprises a second guide slot and a second clamping surface. The second guide slot extends in the second jaw. The second guide slot has an opening segment with a ramped profile and a stapling segment extending generally longitudinally distal of the opening segment. The second jaw is slideably coupled to the distal end of the elongate shaft such that it is movable between a closed position in which the first clamping surface contacts the second clamping surface and a stapling position in which the first clamping surface is parallel to and spaced from the second clamping surface. The second jaw is pivotably coupled to the distal end of the elongate shaft such that the first jaw is pivotable from the closed position to an open position in which the second clamping surface extends at an angle transverse to the first clamping surface. The first guide is slideable in the first guide slot and the second guide is slideable in the second guide slot such that translation of the second guide distally through the open segment of the second guide slot slides and pivots the second jaw from the closed position to the open position, and translation of the second guide distally through the stapling segment positions the second jaw in the stapling position.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of an embodiment of surgical stapling device with the jaws in an open configuration;

FIG. 2 is a perspective view of an embodiment of cartridge including an elongate shaft and a jaw assembly for the surgical stapling device of FIG. 1 with the jaws in a closed configuration;

3

FIG. 3 is a top view of an embodiment of jaw assembly for use in a surgical stapler with the jaws in a closed configuration;

FIG. 4 is a cross-sectional side view of the jaw assembly of FIG. 3;

FIG. 5 is a detailed cross-sectional side view of the jaw assembly of FIG. 3;

FIG. 6 is a detailed cross-sectional end view of the jaw assembly of FIG. 3;

FIG. 7 is a cross-sectional side view of the jaw assembly of FIG. 3 with the jaws in an open configuration;

FIG. 8 is a detailed cross-sectional side view of the jaw assembly of FIG. 3 with the jaws in the open configuration;

FIG. 9 is a cross-sectional side view of the jaw assembly of FIG. 3 with the jaws in a firing configuration;

FIG. 10 is a detailed cross-sectional side view of the jaw assembly of FIG. 3 with the jaws in the firing configuration;

FIG. 11 is a top view of an embodiment of jaw assembly for use in a surgical stapler with the jaws in a closed configuration;

FIG. 12 is a side view of the jaw assembly of FIG. 11;

FIG. 13 is a cross-sectional side view of the jaw assembly FIG. 11;

FIG. 14 is a side view of the jaw assembly of FIG. 11 with the jaws in an open configuration;

FIG. 15 is a cross-sectional side view of the jaw assembly of FIG. 11 with the jaws in the open configuration;

FIG. 16 is a side view of the jaw assembly of FIG. 11 with the jaws in a firing configuration;

FIG. 17 is a cross-sectional side view of the jaw assembly of FIG. 11 with the jaws in a firing configuration;

FIG. 18 is a top view of an embodiment of jaw assembly for use in a surgical stapler with the jaws in a closed configuration;

FIG. 19 is a side view of the jaw assembly of FIG. 18;

FIG. 20 is a cross-sectional side view of the jaw assembly of FIG. 18;

FIG. 21 is a side view of the jaw assembly of FIG. 18 with the jaws in an open configuration;

FIG. 22 is a cross-sectional side view of the jaw assembly FIG. 18 with the jaws in the open configuration;

FIG. 23 is a side view of the jaw assembly of FIG. 18 with the jaws in a firing configuration;

FIG. 24 is a cross-sectional side view of the jaw assembly of FIG. 18 with the jaws in the firing configuration;

FIG. 25 is a top view of an embodiment of jaw assembly for use in the surgical stapler with the jaws in a closed configuration;

FIG. 26 is a side view of the jaw assembly of FIG. 25;

FIG. 27 is a side cross-sectional view of the jaw assembly of FIG. 25;

FIG. 28 is a side view of the jaw assembly of FIG. 25 with the jaws in an open configuration;

FIG. 29 is a side cross-sectional view the jaw assembly FIG. 25 with the jaws in the open configuration;

FIG. 30 is a side view of the jaw assembly of FIG. 25 with the jaws in a firing configuration;

FIG. 31 is a cross-sectional side view of the jaw assembly of FIG. 25 with the jaws in the firing configuration;

FIG. 32 is a top view of an embodiment of jaw assembly for use in a surgical stapler with jaws in a closed configuration;

FIG. 33 is a side view of the jaw assembly of FIG. 32;

FIG. 34 is a cross-sectional side view of the jaw assembly of FIG. 32;

FIG. 35 is a side view of the jaw assembly of FIG. 32 with the jaws in an open configuration;

4

FIG. 36 is a cross-sectional side view of the jaw assembly of FIG. 32 with the jaws in the open configuration;

FIG. 37 is a side view of the jaw assembly of FIG. 32 with the jaws in a firing configuration;

FIG. 38 is a cross-sectional side view of the jaw assembly of FIG. 32 with the jaws in the firing configuration;

#### DETAILED DESCRIPTION OF THE INVENTION

With reference to FIGS. 1-2, an embodiment of surgical stapling device is illustrated. The illustrated embodiment of surgical stapler 10 comprises an elongate shaft 20, a jaw assembly 30, and a handle assembly 40. FIG. 1 illustrates the surgical stapler 10 with the jaw assembly 30 in an open configuration. FIG. 2 illustrates a removable cartridge of the surgical stapler 10 with a jaw assembly 30 in a closed configuration.

With continued reference to FIGS. 1 and 2, the illustrated embodiment of surgical stapler 10 can be sized and configured for use in laparoscopic surgical procedures. For example, the elongate shaft 20 and jaw assembly 30 can be sized and configured to be introduced into a surgical field through an access port or trocar cannula. In some embodiments, the elongate shaft 20 and jaw assembly 30 can be sized and configured to be inserted through a trocar cannula having a relatively small working channel diameter, such as, for example, less than 8 mm. In other embodiments, elongate shaft 20 and jaw assembly 30 can be sized and configured to be inserted through a trocar cannula having a larger working channel diameter, such as, for example, 10 mm, 11 mm, 12 mm, or 15 mm. In other embodiments, it is contemplated that certain aspects of the surgical staplers described herein can be incorporated into a surgical stapling device for use in open surgical procedures.

With continued reference to FIGS. 1 and 2, as illustrated, the elongate shaft 20 comprises a generally tubular member. The elongate shaft 20 extends from a proximal end 22 to a distal end 24. Elongate shaft 20 defines a central longitudinal axis, L, of the surgical stapler 10 extending between the proximal end 22 and the distal end 24.

With continued reference to FIGS. 1 and 2, in the illustrated embodiment, the jaw assembly 30 is coupled to the elongate shaft 20 at the distal end 24 of the elongate shaft 20. The jaw assembly 30 comprises a first jaw 32 and a second jaw 34 pivotally coupled to the first jaw 32. In the illustrated embodiment, the first jaw 32 is fixed to the distal end 24 of elongate shaft 20 such that it extends distally along the central longitudinal axis, L and remains stationary with respect to the elongate shaft 20. In other embodiments, it is contemplated that the jaw assembly 30 is articulable with respect to the elongate shaft 20. In an initial configuration, the first jaw 32 includes a plurality of staples 36 disposed therein. In some embodiments, staples can be initially positioned in the second jaw 34.

With continued reference to FIGS. 1 and 2, in the illustrated embodiment, the jaw assembly 30 can be actuated from an open configuration (FIG. 1) to a closed configuration (FIG. 2) to a stapling configuration by an actuation member or beam that is longitudinally slideable within the elongate shaft. In an initial position, the beam can be positioned at the distal end 24 of the elongate shaft 20. With the beam in the initial position, the second jaw 34 is pivoted away from the first jaw 32 such that the jaw assembly 30 is in the open configuration. The actuation beam engages the second jaw 34 upon translation of the actuation member or beam distally along the longitudinal axis L. Translation of



the actuation beam distally from the initial position a first distance can actuate the jaw assembly from the open configuration to the closed configuration. With the jaw assembly **30** in the closed configuration, the actuation beam can be returned proximally the first distance to return the jaw assembly **30** to the open configuration. A distal end of the actuation beam can advance a staple slider configured to deploy staples from the first jaw **32** such that further translation of the actuation beam distally past the first distance deploys the plurality of staples **36** from the first jaw **32**.

With continued reference to FIGS. **1** and **2**, in the illustrated embodiment, the handle assembly is coupled to the elongate shaft **20** at the proximal end **22** of the elongate shaft **20**. As illustrated, the handle assembly **40** has a pistol grip configuration with a housing defining a stationary handle **42** and a movable handle **44** or trigger pivotably coupled to the stationary handle **42**. It is contemplated that in other embodiments, surgical stapler devices including aspects described herein can have handle assemblies with other configurations such as, for example, scissors-grip configurations, or in-line configurations. As further described in greater detail below, the handle assembly **40** houses an actuation mechanism configured to selectively advance an actuation shaft responsive to movement of the movable handle **44**.

In some embodiments, the surgical stapler **10** can include the plurality of staples **36** positioned in a disposable cartridge while the handle assembly **40** is configured to be reused with multiple staple cartridges. In the illustrated embodiment, the elongate shaft **20** and jaw assembly **30** define a disposable cartridge that is removably coupleable to the handle assembly **40**. Accordingly, in the illustrated embodiment the handle assembly **40** includes a coupler **46** at the distal end thereof. The coupler **46** is adapted to engage the elongate shaft **20** of the surgical stapler **10**. The coupler **46** can be a bayonet connection having an outer connector that can removably couple to handle assembly **42** the elongate shaft **20**, and an inner connector that can removably couple the actuation shaft of the handle assembly **42** to the actuation member of the elongate shaft **20**. Accordingly, the surgical stapler **10** can be configured such that the handle assembly **40** can be reused with multiple disposable cartridges during a surgical procedure. It is contemplated that in other embodiments, the handle assembly and some portion of the elongate shaft can be reusable while a remainder of the elongate shaft in the jaw assembly define a disposable cartridge. In certain other embodiments, the handle assembly and the elongate shaft can be reusable while the jaw assembly defines a disposable cartridge. In still other embodiments, a jaw insert housing a plurality of staples can define a disposable cartridge while the remainder of the surgical stapler is reusable.

As discussed above, surgical staplers **10** described herein can be sized and configured for insertion into a surgical site through a relatively small diameter trocar cannula such as a so-called 5 mm trocar cannula having a working channel inner diameter smaller than about 8 mm. Desirably, jaw assemblies configured for insertion through a 5 mm trocar cannula efficiently employ the relatively limited working space to position both jaws, a plurality of staples, and staple firing elements. In a jaw assembly for a typical laparoscopic surgical stapler, with the jaw assembly in a closed or firing configuration, the first jaw is spaced apart from the second jaw by a gap to accommodate tissue clamped therebetween when the stapler is in use. However, in a jaw assembly configured for insertion through 5 mm trocar cannula, this spacing of the first jaw from the second jaw in the closed position can undesirably be wasted working space. Accord-

ingly, it can be desirable to configure operation of a jaw assembly configured for insertion through a 5 mm trocar cannula such that the gap that would otherwise be wasted working space is repurposed to enhance stapling performance. For example, in a jaw assembly configured to eliminate the gap, the otherwise wasted working space can be repurposed to provide larger staples or more robust staple driving hardware. In various embodiments, jaw assemblies are provided herein that reduce or eliminate the gap between the first jaw and the second jaw in a closed configuration such that the working space of a relatively small diameter surgical stapler can be maximized.

With reference to FIGS. **3-10**, an embodiment of jaw assembly **130** is illustrated. FIG. **3** illustrates a top view of the jaw assembly **130** with the jaws in a closed configuration, and FIGS. **4-6** illustrate cross-sectional views of the jaw assembly **130** in the closed configuration. In the illustrated embodiment, the jaw assembly **130** comprises a first jaw **102** having a first clamping surface **104**, a second jaw **106** having a second clamping surface **108**, and a link **112**. The first jaw **102** extends distally from the distal end **24** of the elongate shaft **20** (FIGS. **1-2**) and is fixed to the elongate shaft **20**. The second jaw **106** is pivotably coupled to the first jaw **102**. In the illustrated embodiment, the second jaw **106** is pivotably coupled to the distal end **24** of the elongate shaft **20** by the link **112**. For example, the link **112** can extend from a proximal end, which is pivotably coupled to the distal end **24** of the elongate shaft **20**, such as with a pinned connection to a distal end, which is pivotably coupled to the second jaw **106**, such as with a pinned connection.

An actuation mechanism is operably coupled to the handle assembly **40** and actuatable by the movable trigger **44** to actuate the jaw assembly **130** in an open/closed mode, in a firing mode, and in a reverse mode. The jaws **102**, **106** of the jaw assembly **130** are thus actuatable between a closed configuration in which the first clamping surface **104** of the first jaw **102** is in contact with or is immediately adjacent to the second clamping surface **108** of the second jaw **106**, an open configuration in which the second clamping surface **108** extends at an angle transverse to the longitudinal axis **L** away from the first clamping surface **104**, and a stapling or firing configuration in which the second clamping surface **108** is substantially parallel to the first clamping surface **104** and is spaced therefrom. With the jaws in the stapling or firing configuration, a plurality of staples can be deployed from the first jaw **102** through tissue positioned between the first and second jaws **102**, **106** and formed against the second clamping surface **108** of the second jaw **106**. In some embodiments, the actuation mechanism includes an actuation member such as an actuation beam **150** that is longitudinally slideable in the elongate shaft **20**. The actuation beam **150** can include a first guide **114** and a second guide **116** formed thereon.

With reference to FIG. **6**, in some embodiments, a distal end of the actuation beam **150** comprises an 'I-beam' cross sectional profile with the first and second guides **114**, **116** being defined by the horizontal segments of the 'I,' and the vertical segment of the 'I' comprising the actuation beam **150**. In other embodiments, the actuation member or beam can have another guide configuration. For example, the guides can comprise posts, tabs, or other projections extending from the actuation member.

With reference to FIGS. **4-5**, the first jaw **102** can comprise a first guide slot **118** configured to receive the first guide **114** of the actuation beam **150** in sliding engagement.

As illustrated, the first guide slot **118** can extend generally longitudinally distally from the distal end **24** of the elongate shaft **20**.

With continued reference to FIGS. **4-5**, in the illustrated embodiment, the link **112** can comprise a second guide slot **120** formed therein. The second guide slot **120** can extend from a proximal end to a distal end of the link **112** and can include an initial closed segment at the proximal end of the link **112**, an opening segment distal the closed segment, and a firing transition segment at the distal end of the link **112**.

With reference to FIGS. **4-8**, the open segment has a curved or angular profile oriented such that distal sliding of the second guide **116** through the second guide slot **120** distal of the initial closed segment pivots the link **112** (and the second jaw **106** pivotably coupled thereto) away from the first jaw **102** to actuate the jaw assembly **130** from an initial closed position in which the jaw assembly has a relatively low diameter for insertion into a surgical port to an open position for receiving tissue between the first and second jaws **102**, **106**. In some embodiments, the link **112** can be biased away from the first jaw **102**. For example, as illustrated, the jaw assembly **130** can comprise at least one spring **160** biasing the link **112** away from the first jaw **102**. This bias can tend to engage the second guide **116** with the opening segment of the second guide slot **120** and position the second jaw **106** in the open position (FIGS. **7-8**).

With reference to FIGS. **9-10**, once tissue has been positioned between the first jaw **102** and the second jaw **106** in the open configuration at a desired stapling position, the actuation member **150** can be further advanced distally to position the jaws **102**, **106** of the jaw assembly **130** in a stapling or firing configuration. Further distal movement of the actuation beam **150** advances the second guide **116** over the firing transition segment of the second guide slot **120** of the link **112** to pivot the second jaw to a position spaced apart from the first jaw a predetermined distance. The predetermined distance can be selected based on a desired tissue type for stapling in a procedure or a given staple geometry. Further distal movement of the actuation member **150** causes the second guide **116** to be received in a third guide slot **122** disposed in the second jaw **106**. The third guide slot **122** can include a chamfer, radiused edge, or another transition feature to facilitate the translation of the second guide **116** distally from the second guide slot **120** to the third guide slot **122**. Movement of the second guide **116** over the transition feature can further pivot the second jaw **106** such that the second clamping surface **108** is parallel to the first clamping surface **104**.

As illustrated, the third guide slot **122** extends generally longitudinally along the second jaw **106** generally parallel to the second clamping surface **108** such that further distal advancement of the second guide **116** within the third guide slot **122** maintains the parallel orientation of the first and second clamping surfaces **104**, **108** in the firing configuration. In other embodiments, it is contemplated that the third guide slot can extend along a curvilinear path or a path extending transversely to the second clamping surface **108** to generate a clamping force between the first and second clamping surfaces **104**, **108** as the actuation member **150** is advanced distally.

With reference to FIGS. **9-10**, in some embodiments, a distal end of the actuation member **150** can engage a staple driver. As the actuation member **150** is advanced distally with the jaws **102**, **106** of the jaw assembly **130** in the firing position, the staple driver can deploy staples from the first

jaw **102**. The staple driver can include a cutting blade configured to cut tissue between rows of staples deployed by the jaw assembly.

With reference to FIGS. **11-17**, another embodiment of jaw assembly **230** for use with a surgical stapler **10** is illustrated. In the illustrated embodiment, the jaw assembly **230** comprises a first jaw **202** having a first clamping surface **204** and comprising a first guide slot **218**, a link **212** comprising a second guide slot **220**, and a second jaw **206** having a second clamping surface **208** and comprising a third guide slot **222**. An actuation member **250** or beam comprising a first guide **214** and a second guide **216** can actuate the jaw assembly **230** from the closed configuration (FIGS. **11-13**), to the open configuration (FIGS. **14-15**) to the firing or stapling configuration (FIGS. **16-17**) in a sequence of operation substantially as described above with respect to the jaw assembly **130** of FIGS. **3-10**.

With reference to FIG. **14**, unlike the jaw assembly **130** of FIGS. **3-10**, the second jaw **206** of the jaw assembly **230** is directly biased away from the first jaw **202**. For example, in the illustrated embodiment a spring **260** is coupled to the first jaw **202** and the second jaw **206** to bias the second jaw **206** away from the first jaw. Additionally, the jaw assembly **230** includes a pivotal stop preventing excess pivoting of the second jaw **206** relative to the first jaw **202**. In the illustrated embodiment, the second jaw **206** can comprise an extension such as an arm that extends proximally past the pivotal coupling of the second jaw **206** to the link **212**. The extension can be sized and configured to engage the first jaw **202** when the jaw assembly **230** is positioned in the open configuration to interfere with further pivoting of the second jaw **206** away from the first jaw **202**.

With reference to FIGS. **18-24**, an embodiment of jaw assembly **330** for use with a surgical stapler **10** having a sliding pivot point is illustrated. In the illustrated embodiment, the jaw assembly **330** comprises a first jaw **302** having a first clamping surface **304** and comprising a first guide slot **318** and a second jaw **306** having a second clamping surface **308** and comprising a second guide slot **320**. An actuation member **350** or beam comprising a first guide **314** and a second guide **316** can actuate the jaw assembly **330** from the closed configuration (FIGS. **18-20**), to the open configuration (FIGS. **21-22**) to the firing or stapling configuration (FIGS. **23-24**) in a sequence of operation similar to those described above with respect to the jaw assemblies **130**, **230**.

With reference to FIGS. **20-23**, in the illustrated embodiment of jaw assembly **330**, the second jaw **306** is coupled to the first jaw **302** without an intercoupled link **112**, **212** therebetween. Rather, the jaw assembly **330** includes a sliding pivot joint **312** that allows the second jaw **306** to pivot about a point that is translatable with respect to the first jaw **302**. For example, the sliding pivot joint **312** can comprise a pivoting pin disposed in a slot formed in the first jaw **302**.

With continued reference to FIGS. **20-23**, the second guide slot **320** disposed in the second jaw **306** can comprise an opening segment adjacent a proximal end of the second guide slot and a firing transition segment distal the opening segment. Distal movement of the actuation member **350** distally advances the second guide **316** along the opening segment of the second guide slot **320** to slide the second jaw **306** away from the first jaw **302** and pivot the second jaw **306** into the open configuration (FIGS. **21-22**). Further distal movement of the actuation member distally advances the second guide **316** past the firing transition segment and into a firing segment extending generally longitudinally along

the second jaw **306** to position the jaw assembly **330** in a firing configuration (FIGS. **23-24**).

With reference to FIG. **25-31**, an embodiment of jaw assembly **430** with a slotted actuator for use in a surgical stapler **10** is illustrated. In the illustrated embodiment, the jaw assembly **430** comprises a first jaw **402** having a first clamping surface **404** and comprising a first guide slot **418**, a link **412**, and a second jaw **406** having a second clamping surface **408** and comprising a second guide slot **420**. An actuation member **450** or beam comprising a first guide **414** and a second guide **416** can actuate the jaw assembly **430** from the closed configuration (FIGS. **25-27**), to the open configuration (FIGS. **28-29**) to the firing or stapling configuration (FIGS. **30-31**) in a sequence of operation similar to those described above with respect to the jaw assemblies **130**, **230**.

With reference to FIGS. **27-29**, the link **412** can include a third guide **426** thereon, such as one or more pins, tabs, or posts extending therefrom. The actuation member **450** can include a third guide slot **424** formed therein. The third guide **426** of the link **412** can be slideably engaged in the third guide slot **424**. The third guide slot **424** can comprise an opening segment and a firing transition segment which extend transverse to the longitudinal axis. When the actuation member **450** is advanced distally from an initial position, the third guide **426** of the link **412** passes through the opening segment such that the link **412** is pivoted away from the first jaw **402** (FIGS. **28-29**). Continued translation of the actuation member **450** advances the third guide **426** of the link **412** past the firing transition segment of the third guide slot **424** to position the second jaw **406** in the firing position (FIGS. **30-31**).

With reference to FIGS. **32-38**, another embodiment of jaw assembly **530** for use with a surgical stapler **10** is illustrated. In the illustrated embodiment, the jaw assembly **530** comprises a first jaw **502** having a first clamping surface **504** and comprising a first guide slot **518**, a link **512** comprising a second guide slot **520**, and a second jaw **506** having a second clamping surface **508** and comprising a third guide slot **522**. An actuation member **550** or beam comprising a first guide **514** and a second guide **516** can actuate the jaw assembly **530** from the closed configuration (FIGS. **32-34**), to the open configuration (FIGS. **35-36**) to the firing or stapling configuration (FIGS. **37-38**) in a sequence of operation similar to those described above with respect to the jaw assemblies **130**, **230**, **430**.

With reference to FIGS. **34-36**, in the illustrated embodiment, the actuation member **550** can include a first guide **514** positioned at a distal end of a first arm or extension and a second guide positioned at a distal end of a second arm or extension. The first and second arms can be flexibly coupled to one another such that a distance between the first guide **514** and the second guide **516** can be varied. The first and second arms can be biased away from one another. Advantageously, the variable spacing of the first guide **514** and second guide **516** can allow positioning of the third guide slot **522** in a position relatively close to an outer surface opposite the second clamping surface **508** of the second jaw **506**. Accordingly, additional working space in the second jaw adjacent the second clamping surface can be freed by positioning the third guide slot **522** closer to the outer surface.

Although this application discloses certain preferred embodiments and examples, it will be understood by those skilled in the art that the present inventions extend beyond the specifically disclosed embodiments to other alternative embodiments and/or uses of the invention and obvious

modifications and equivalents thereof. Further, the various features of these inventions can be used alone, or in combination with other features of these inventions other than as expressly described above. Thus, it is intended that the scope of the present inventions herein disclosed should not be limited by the particular disclosed embodiments described above, but should be determined only by a fair reading of claims which follow.

What is claimed is:

1. A surgical stapler comprising:

an elongate shaft having a proximal end and a distal end and defining a longitudinal axis between the proximal end and the distal end;

a handle assembly disposed at the proximal end of the elongate shaft;

an actuation mechanism actuatable by the handle assembly, the actuation mechanism comprising an actuation beam extending through at least a portion of the elongate shaft;

a jaw assembly disposed at the distal end of the elongate shaft, the jaw assembly comprising:

a first jaw defining a first clamping surface;

a second jaw defining a second clamping surface; and

a plurality of staples positioned in the first jaw;

wherein the jaw assembly is actuatable by longitudinal movement of the actuation beam between a closed position in which the first clamping surface contacts the second clamping surface, an open position in which the second clamping surface extends at an angle transverse to the first clamping surface, and a stapling position in which the first clamping surface extends parallel to the second clamping surface and is spaced apart from the second clamping surface, and

wherein the jaw assembly further comprises a link having a proximal end pivotably coupled to the proximal end of the elongate shaft and a distal end pivotably coupled to the second jaw.

2. A surgical stapler comprising:

an elongate shaft having a proximal end and a distal end and defining a longitudinal axis between the proximal end and the distal end;

a handle assembly disposed at the proximal end of the elongate shaft;

an actuation mechanism actuatable by the handle assembly, the actuation mechanism comprising an actuation member extending through at least a portion of the elongate shaft, the actuation member comprising a first guide and a second guide thereon;

a jaw assembly disposed at the distal end of the elongate shaft, the jaw assembly comprising:

a first jaw extending distally from the distal end of the elongate shaft, the first jaw comprising a first guide slot extending longitudinally therein;

a link having a proximal end and a distal end, the link comprising a second guide slot having a ramped opening profile formed therein, and the proximal end of the link being pivotably coupled to the distal end of the elongate shaft;

a second jaw extending distally from the distal end of the link and pivotably coupled to the distal end of the link, the second jaw comprising a third guide slot extending longitudinally therein; and

a plurality of staples disposed in the first jaw;

wherein the first guide is slideable in the first guide slot and the second guide is slideable in the second guide slot and the third guide slot, and wherein translation of the second guide distally over the ramped opening

profile of the second guide slot pivots the link away from the first jaw to define an open position of the jaw assembly.

3. The surgical stapler of claim 2, wherein the link is pivotally biased away from the first jaw. 5

4. The surgical stapler of claim 3, wherein the second jaw is pivotally biased towards the first jaw.

5. The surgical stapler of claim 4, wherein the link and the second jaw are configured to interfere with pivotal motion of the second jaw with respect to the link to limit pivoting of 10 the second jaw towards the first jaw.

\* \* \* \* \*