



US0D1005764S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,005,764 S**
Salus (45) **Date of Patent:** **** Nov. 28, 2023**

(54) **SIDE RAIL FOR BED**

(71) Applicant: **LINET SPOL. S R.O.**, Slany (CZ)

(72) Inventor: **Michal Salus**, Roudnice nad Labem (CZ)

(73) Assignee: **LINET SPOL. S R.O.**, Slany (CZ)

(**) Term: **15 Years**

(21) Appl. No.: **29/803,258**

(22) Filed: **Aug. 11, 2021**

(30) **Foreign Application Priority Data**

Feb. 11, 2021 (EM) 008432090-0001

Feb. 11, 2021 (EM) 008432090-0002

(Continued)

(51) **LOC (14) Cl.** **06-06**

(52) **U.S. Cl.**

USPC **D6/718.3; D24/184**

(58) **Field of Classification Search**

USPC D6/382, 390, 391, 392, 718, 718.13,
D6/718.3; D24/183, 184

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D427,465 S * 7/2000 Thom D6/718

D616,678 S * 6/2010 Heimbrock D6/718.3

(Continued)

FOREIGN PATENT DOCUMENTS

EM 007059704-0002 * 12/2019

EM 007059704-0003 * 12/2019

(Continued)

OTHER PUBLICATIONS

Generic, "Medical Hospital ICU Bed", first available Jan. 8, 2021
<https://www.amazon.ca/Medical-Hospital-Electric-Adjustable-GM->

7006/dp/B08T9X1WV7/ref=sr_1_148?crd=3I8PK4DL6YBEQ
&keywords=hospital+bed&qid=1684884983&sprefix=hospital+bed%
2Caps%2C115&sr=8-148 (Year: 2021).*

(Continued)

Primary Examiner — Bao-Yen T Nguyen

Assistant Examiner — Jessica Ruth Grable

(74) *Attorney, Agent, or Firm* — Thedford I. Hitaffer;
Hitaffer & Hitaffer, PLLC

(57) **CLAIM**

The ornamental design for a side rail for bed, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a side rail for bed taken from the left side thereof.

FIG. 2 is a front perspective view of the side rail for bed shown in FIG. 1 taken from the right side thereof.

FIG. 3 is a front elevational view of the side rail for bed shown in FIG. 1.

FIG. 4 is a rear elevational view of the side rail for bed shown in FIG. 1.

FIG. 5 is a top plan view of the side rail for bed shown in FIG. 1.

FIG. 6 is a right side elevational view of the side rail for bed shown in FIG. 1.

FIG. 7 is a left side elevational view of the side rail for bed shown in FIG. 1.

FIG. 8 is a front perspective view of another side rail for bed taken from the right side thereof.

FIG. 9 is a front perspective view of the side rail for bed shown in FIG. 8 taken from the left side thereof.

FIG. 10 is a front elevational view of the side rail for bed shown in FIG. 8.

FIG. 11 is a rear elevational view of the side rail for bed shown in FIG. 8.

FIG. 12 is a top plan view of the side rail for bed shown in FIG. 8.

FIG. 13 is a right side elevational view of the side rail for bed shown in FIG. 8; and,

(Continued)

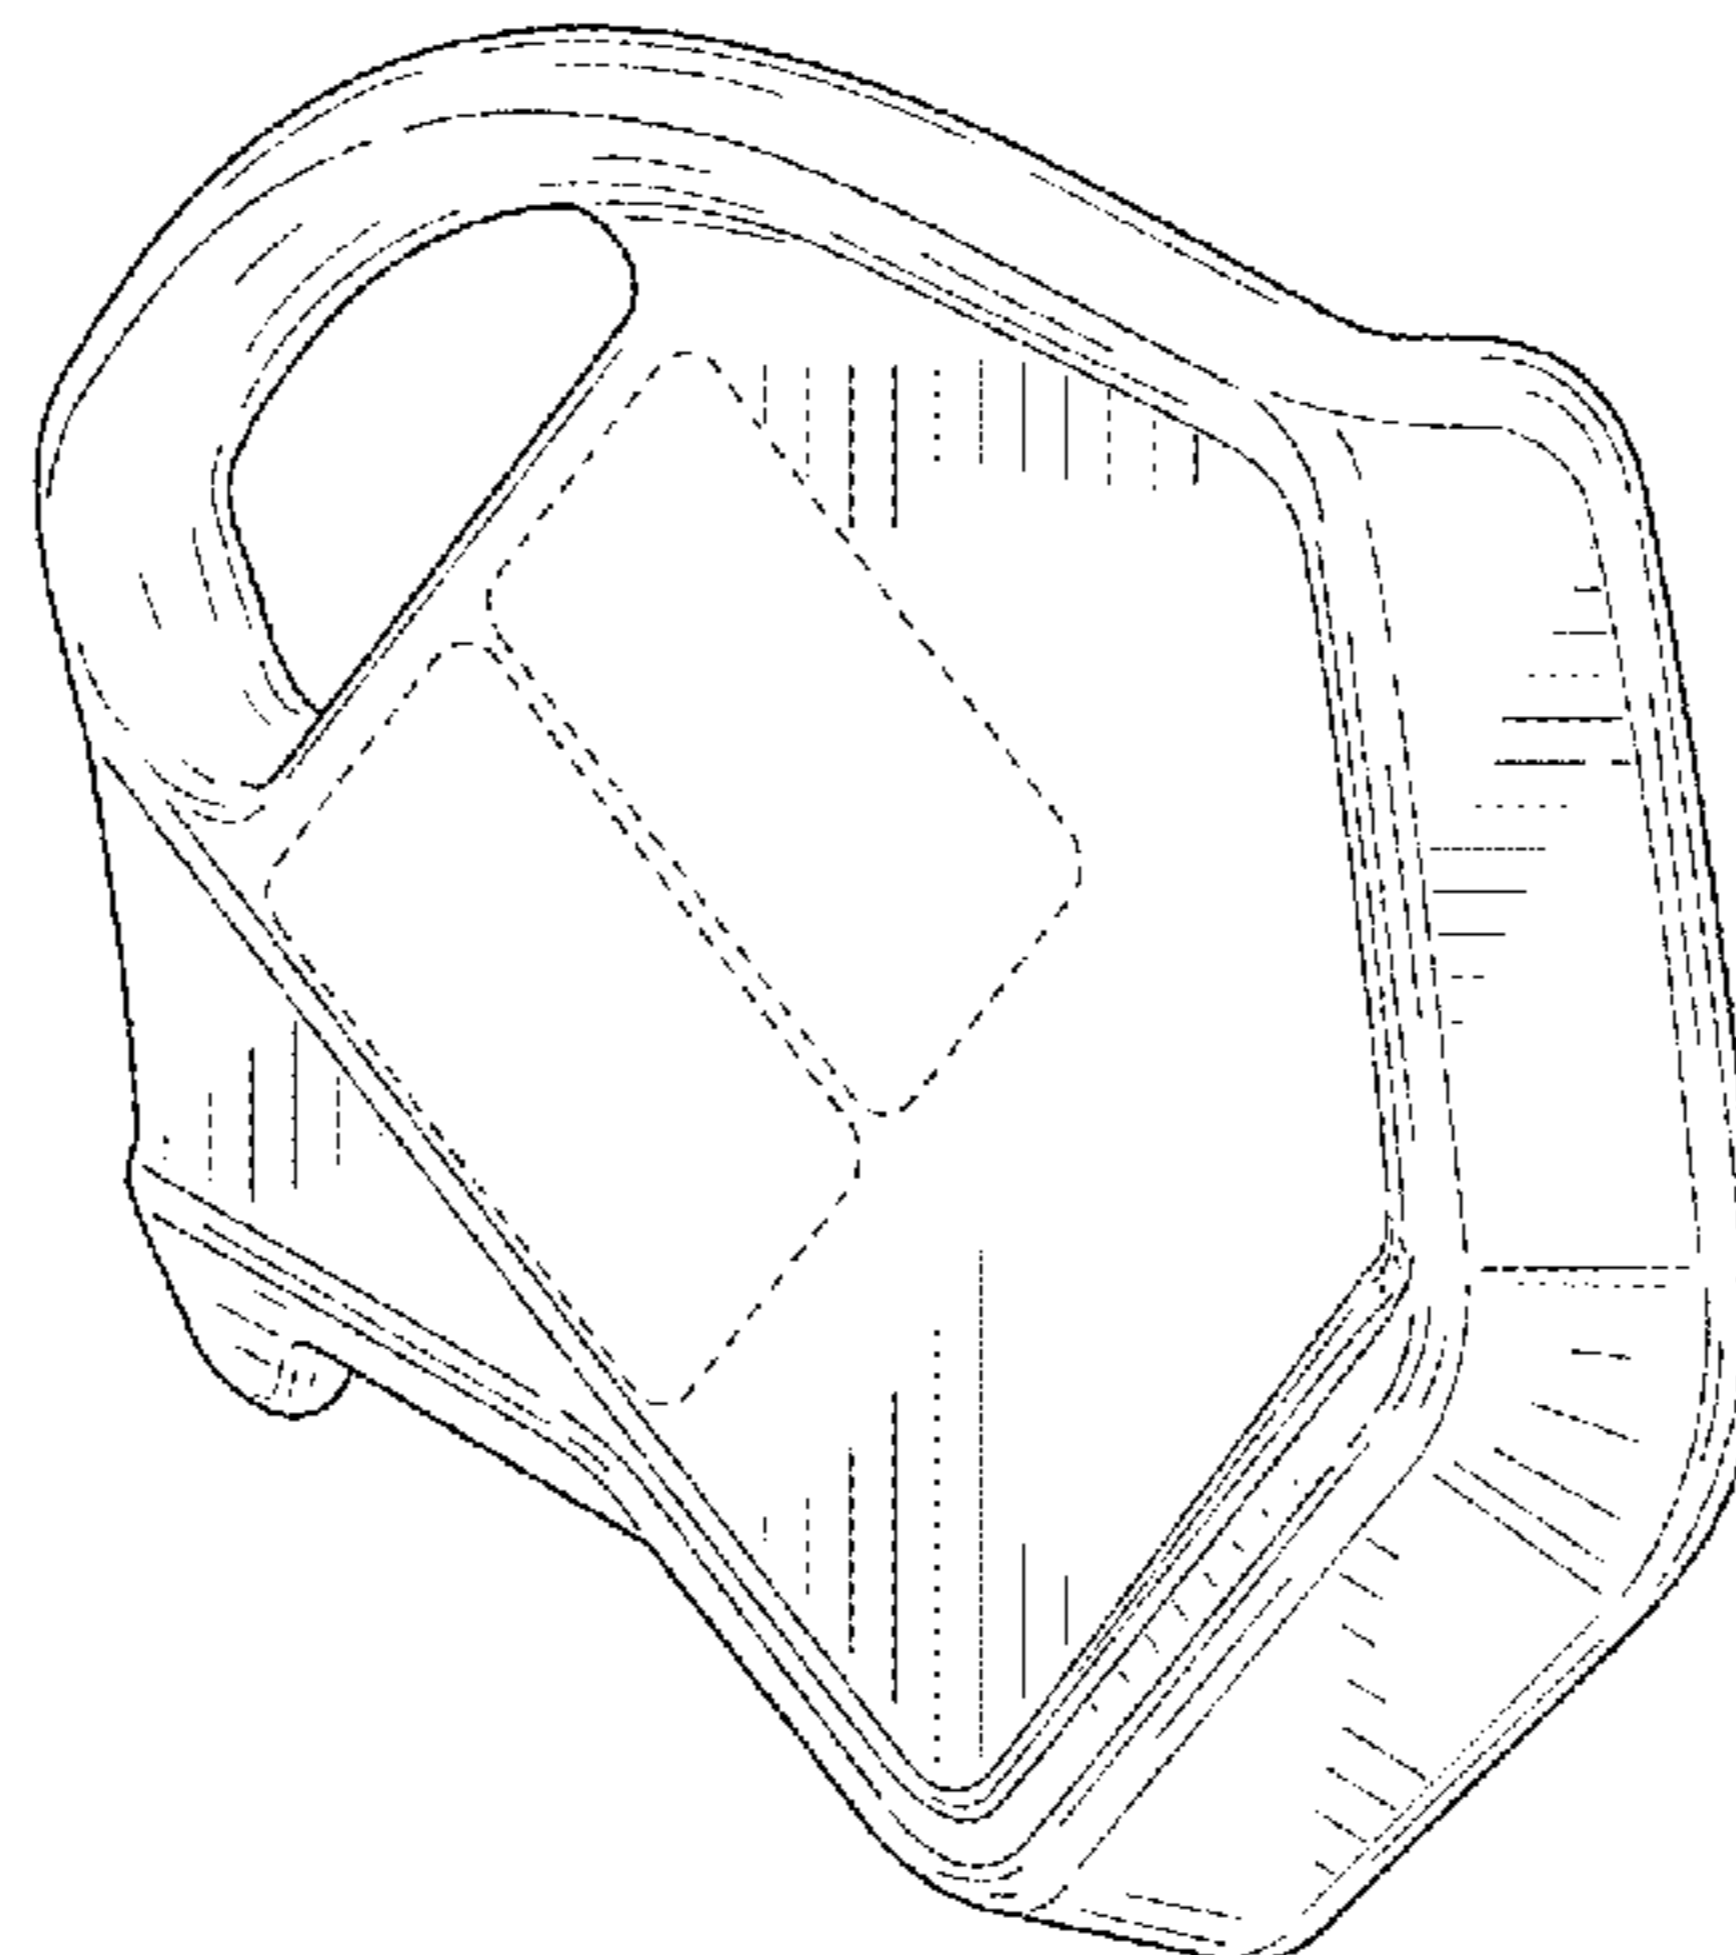


FIG. 14 is a left side elevational view of the side rail for bed shown in FIG. 8.

The broken lines represent portions of the bed and form no part of the claimed design.

1 Claim, 6 Drawing Sheets

(30) Foreign Application Priority Data

Feb. 11, 2021 (EM) 008432090-0003
 Feb. 11, 2021 (EM) 008432090-0004

(58) Field of Classification Search

CPC A47C 17/04; A47C 21/08; A61G 7/00;
 A61G 7/0507; A61G 7/0514; A61G 7/015
 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D616,679 S * 6/2010 Heimbrock D6/718.3
 D617,586 S * 6/2010 Heimbrock D6/718.3
 D617,587 S * 6/2010 Heimbrock D6/718.3
 D617,588 S * 6/2010 Heimbrock D6/718.3
 D617,589 S * 6/2010 Heimbrock D6/718.3
 D627,985 S * 11/2010 Salus D6/391
 D628,416 S * 12/2010 Heimbrock D6/718.3
 D637,018 S * 5/2011 Heimbrock D6/718.3
 D637,019 S * 5/2011 Heimbrock D6/718.3
 D637,020 S * 5/2011 Heimbrock D6/718.3
 D640,887 S * 7/2011 Heimbrock D6/718.3
 D646,079 S * 10/2011 York D6/391
 D668,087 S * 10/2012 Fejt D6/718
 8,621,688 B2 * 1/2014 Andrienko A61G 7/015
 5/426
 8,677,535 B2 * 3/2014 Turner A61G 7/053
 5/602
 D707,480 S * 6/2014 Heimbrock D6/392
 D707,483 S * 6/2014 Heimbrock D6/718.3

8,745,786 B2 * 6/2014 Andrienko A61G 7/0524
 5/426
 D710,507 S * 8/2014 Leng D24/183
 D769,042 S * 10/2016 O'Neal D6/718.3
 D770,824 S * 11/2016 O'Neal D6/392
 D804,882 S * 12/2017 Zerhusen D6/718.3
 D804,883 S * 12/2017 Zerhusen D6/718.3
 D819,382 S * 6/2018 O'Neal D6/718.3
 D825,973 S * 8/2018 O'Neal D6/718.3
 D850,836 S * 6/2019 Zerhusen D6/718.3
 D858,166 S * 9/2019 Zerhusen D6/718.3
 2006/0107460 A1 * 5/2006 Wiggins A61G 7/0514
 5/430
 2009/0113633 A1 * 5/2009 Hayes A61G 7/0507
 5/619
 2012/0110735 A1 * 5/2012 Andrienko A61G 7/0507
 5/430
 2012/0144587 A1 * 6/2012 Andrienko A61G 7/015
 5/618
 2013/0117934 A1 * 5/2013 Heimbrock A61G 7/0514
 5/430
 2016/0058640 A1 * 3/2016 Morin A61G 7/0507
 5/430
 2017/0172829 A1 * 6/2017 Tessmer A61G 7/0516
 2019/0290517 A1 * 9/2019 Ross A61G 7/0508

FOREIGN PATENT DOCUMENTS

IN 309516-0001 * 9/2018
 JP D1127439 * 11/2001

OTHER PUBLICATIONS

HopeFull Store, "Fully Electric ICU Hospital Bed", first available Jul. 11, 2018 <https://www.amazon.com/Hopefull-Function-Electric-Hospital-Mattress/dp/B083PZ7JFN> (Year: 2018).
 FC-Bed, "Hospital Intensive Care Medical Bed" first avail Jul. 27, 2021 https://www.amazon.ca/Intensive-Motorised-Electrical-Trendelenburg-Reverse-Trendelenburg/dp/B09B9S8V5G/ref=sr_1_11?crd=3PSP5O45E1DWS&keywords=ICU+bed+rails&qid=1686046059&srefix=icu+bed+rails%2Caps%2C87&sr=8-11 (Year: 2021).*

* cited by examiner

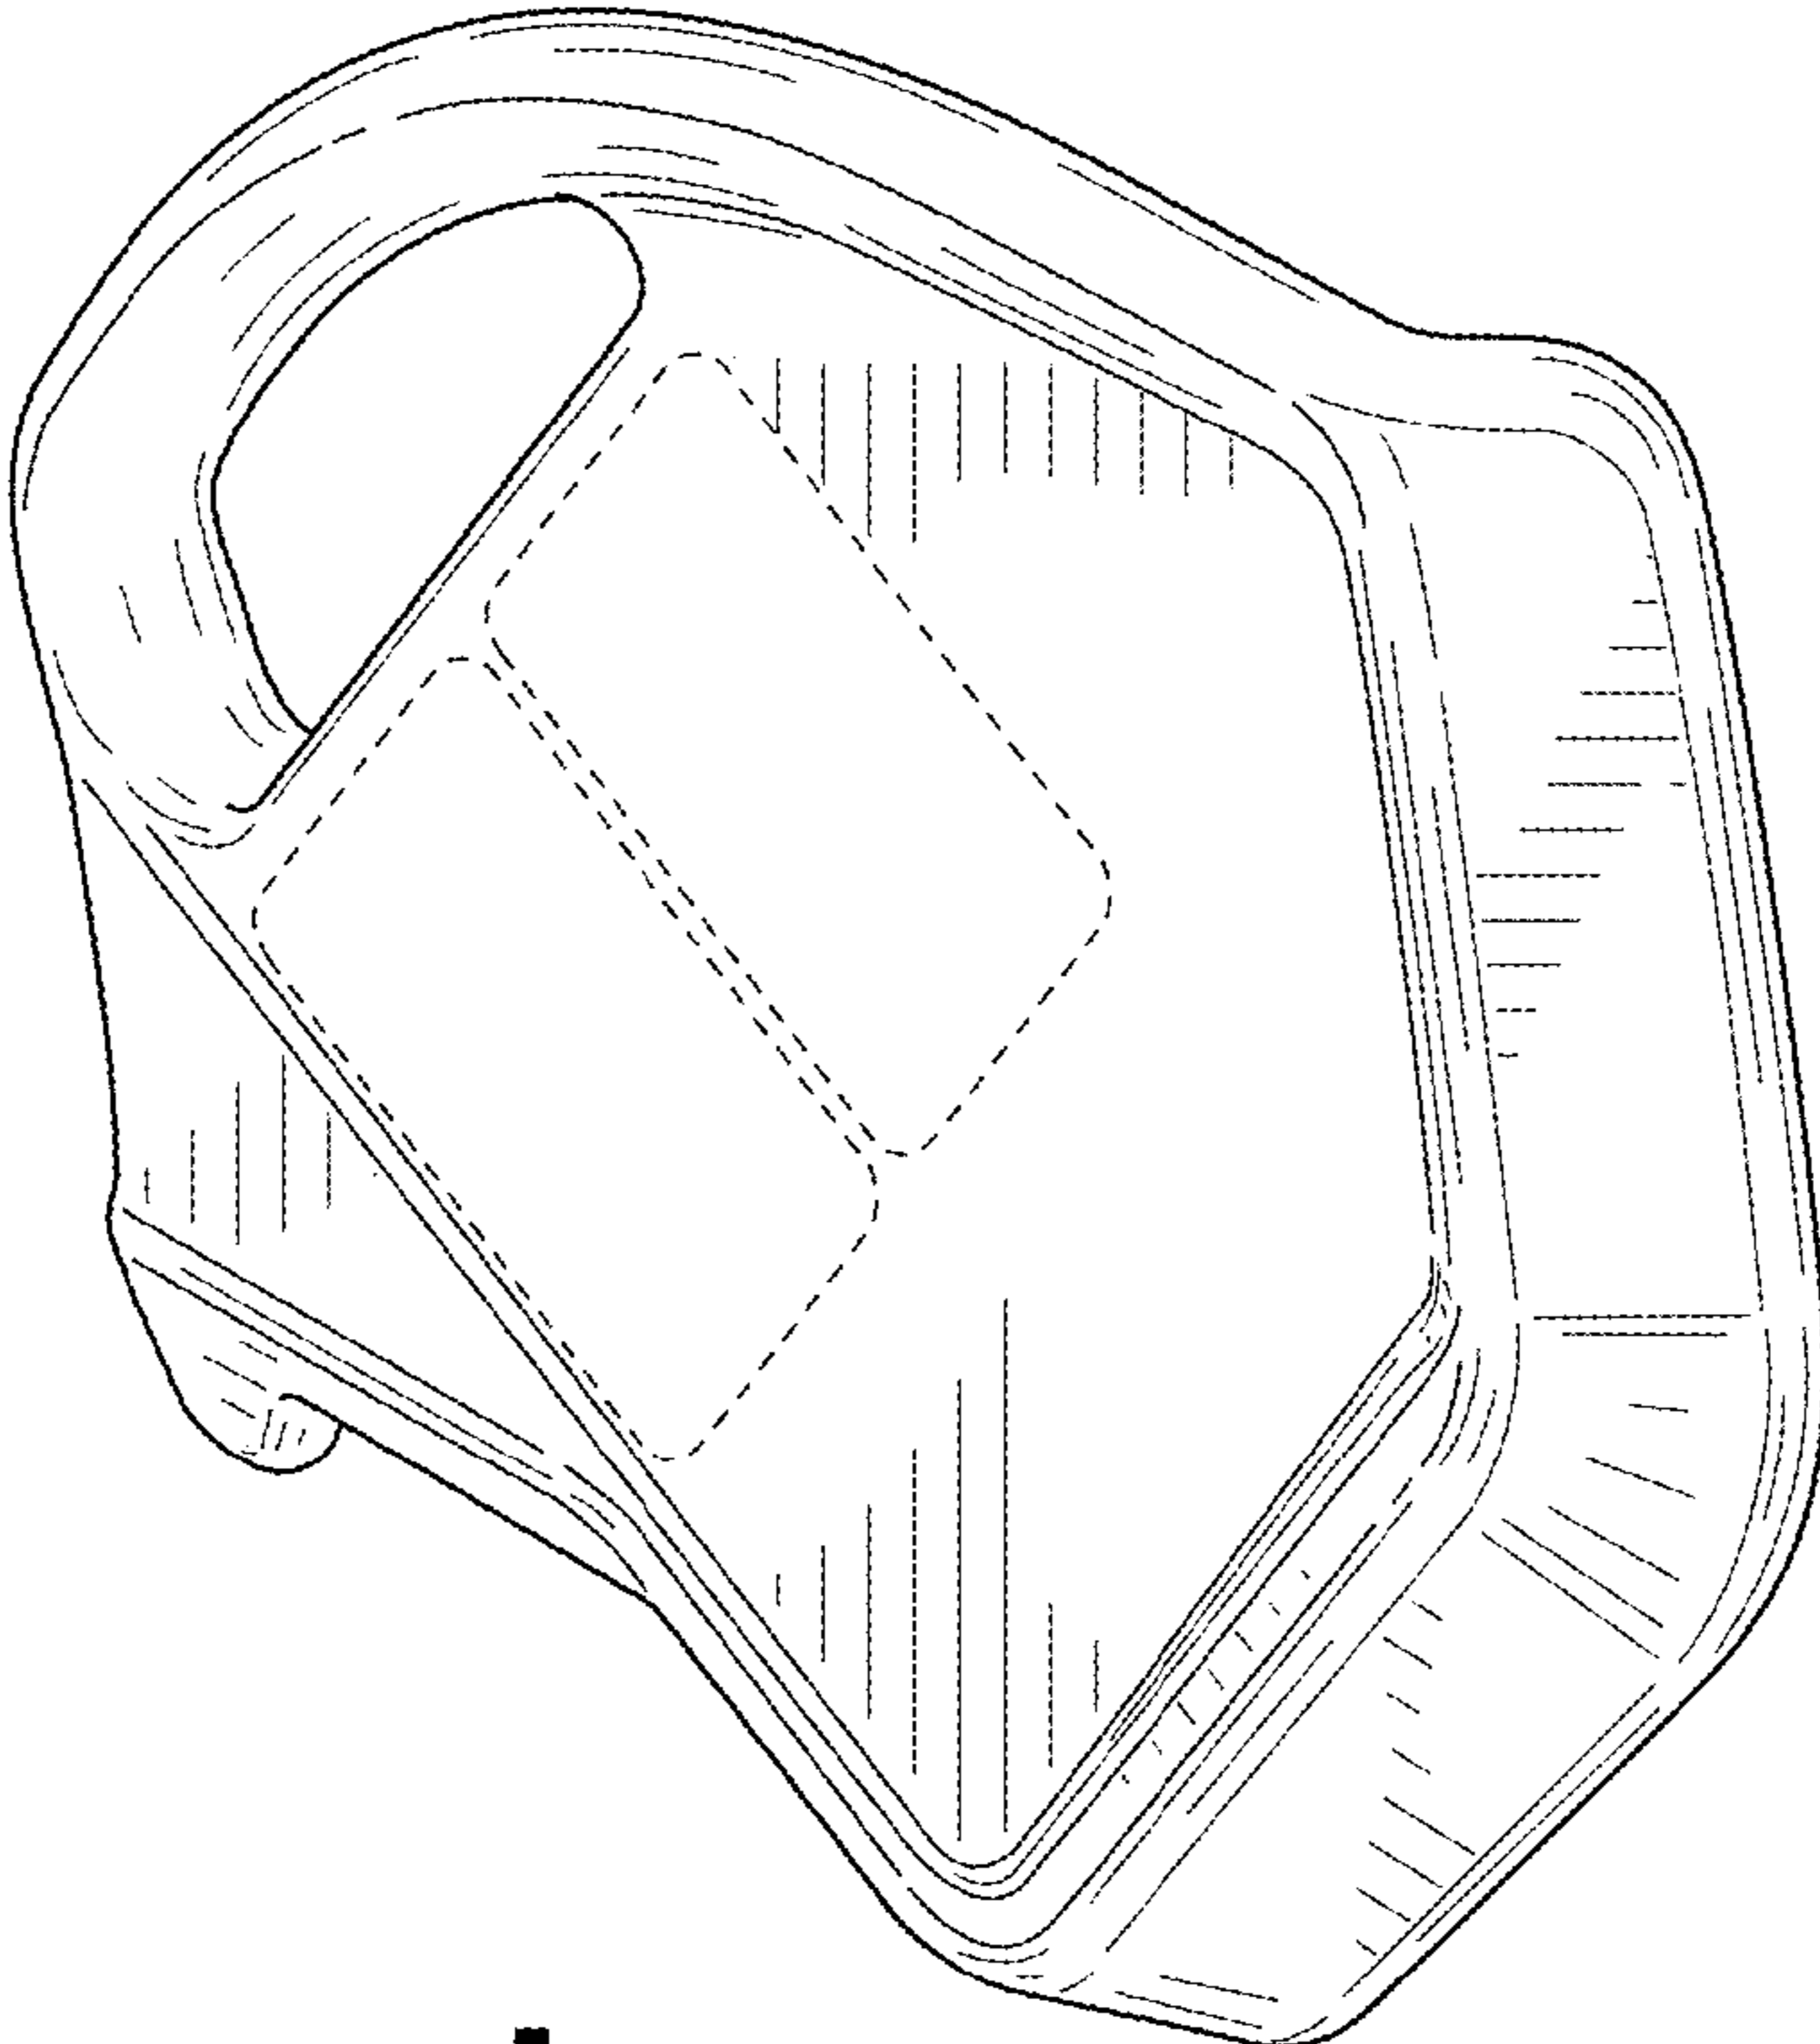


FIG. 1

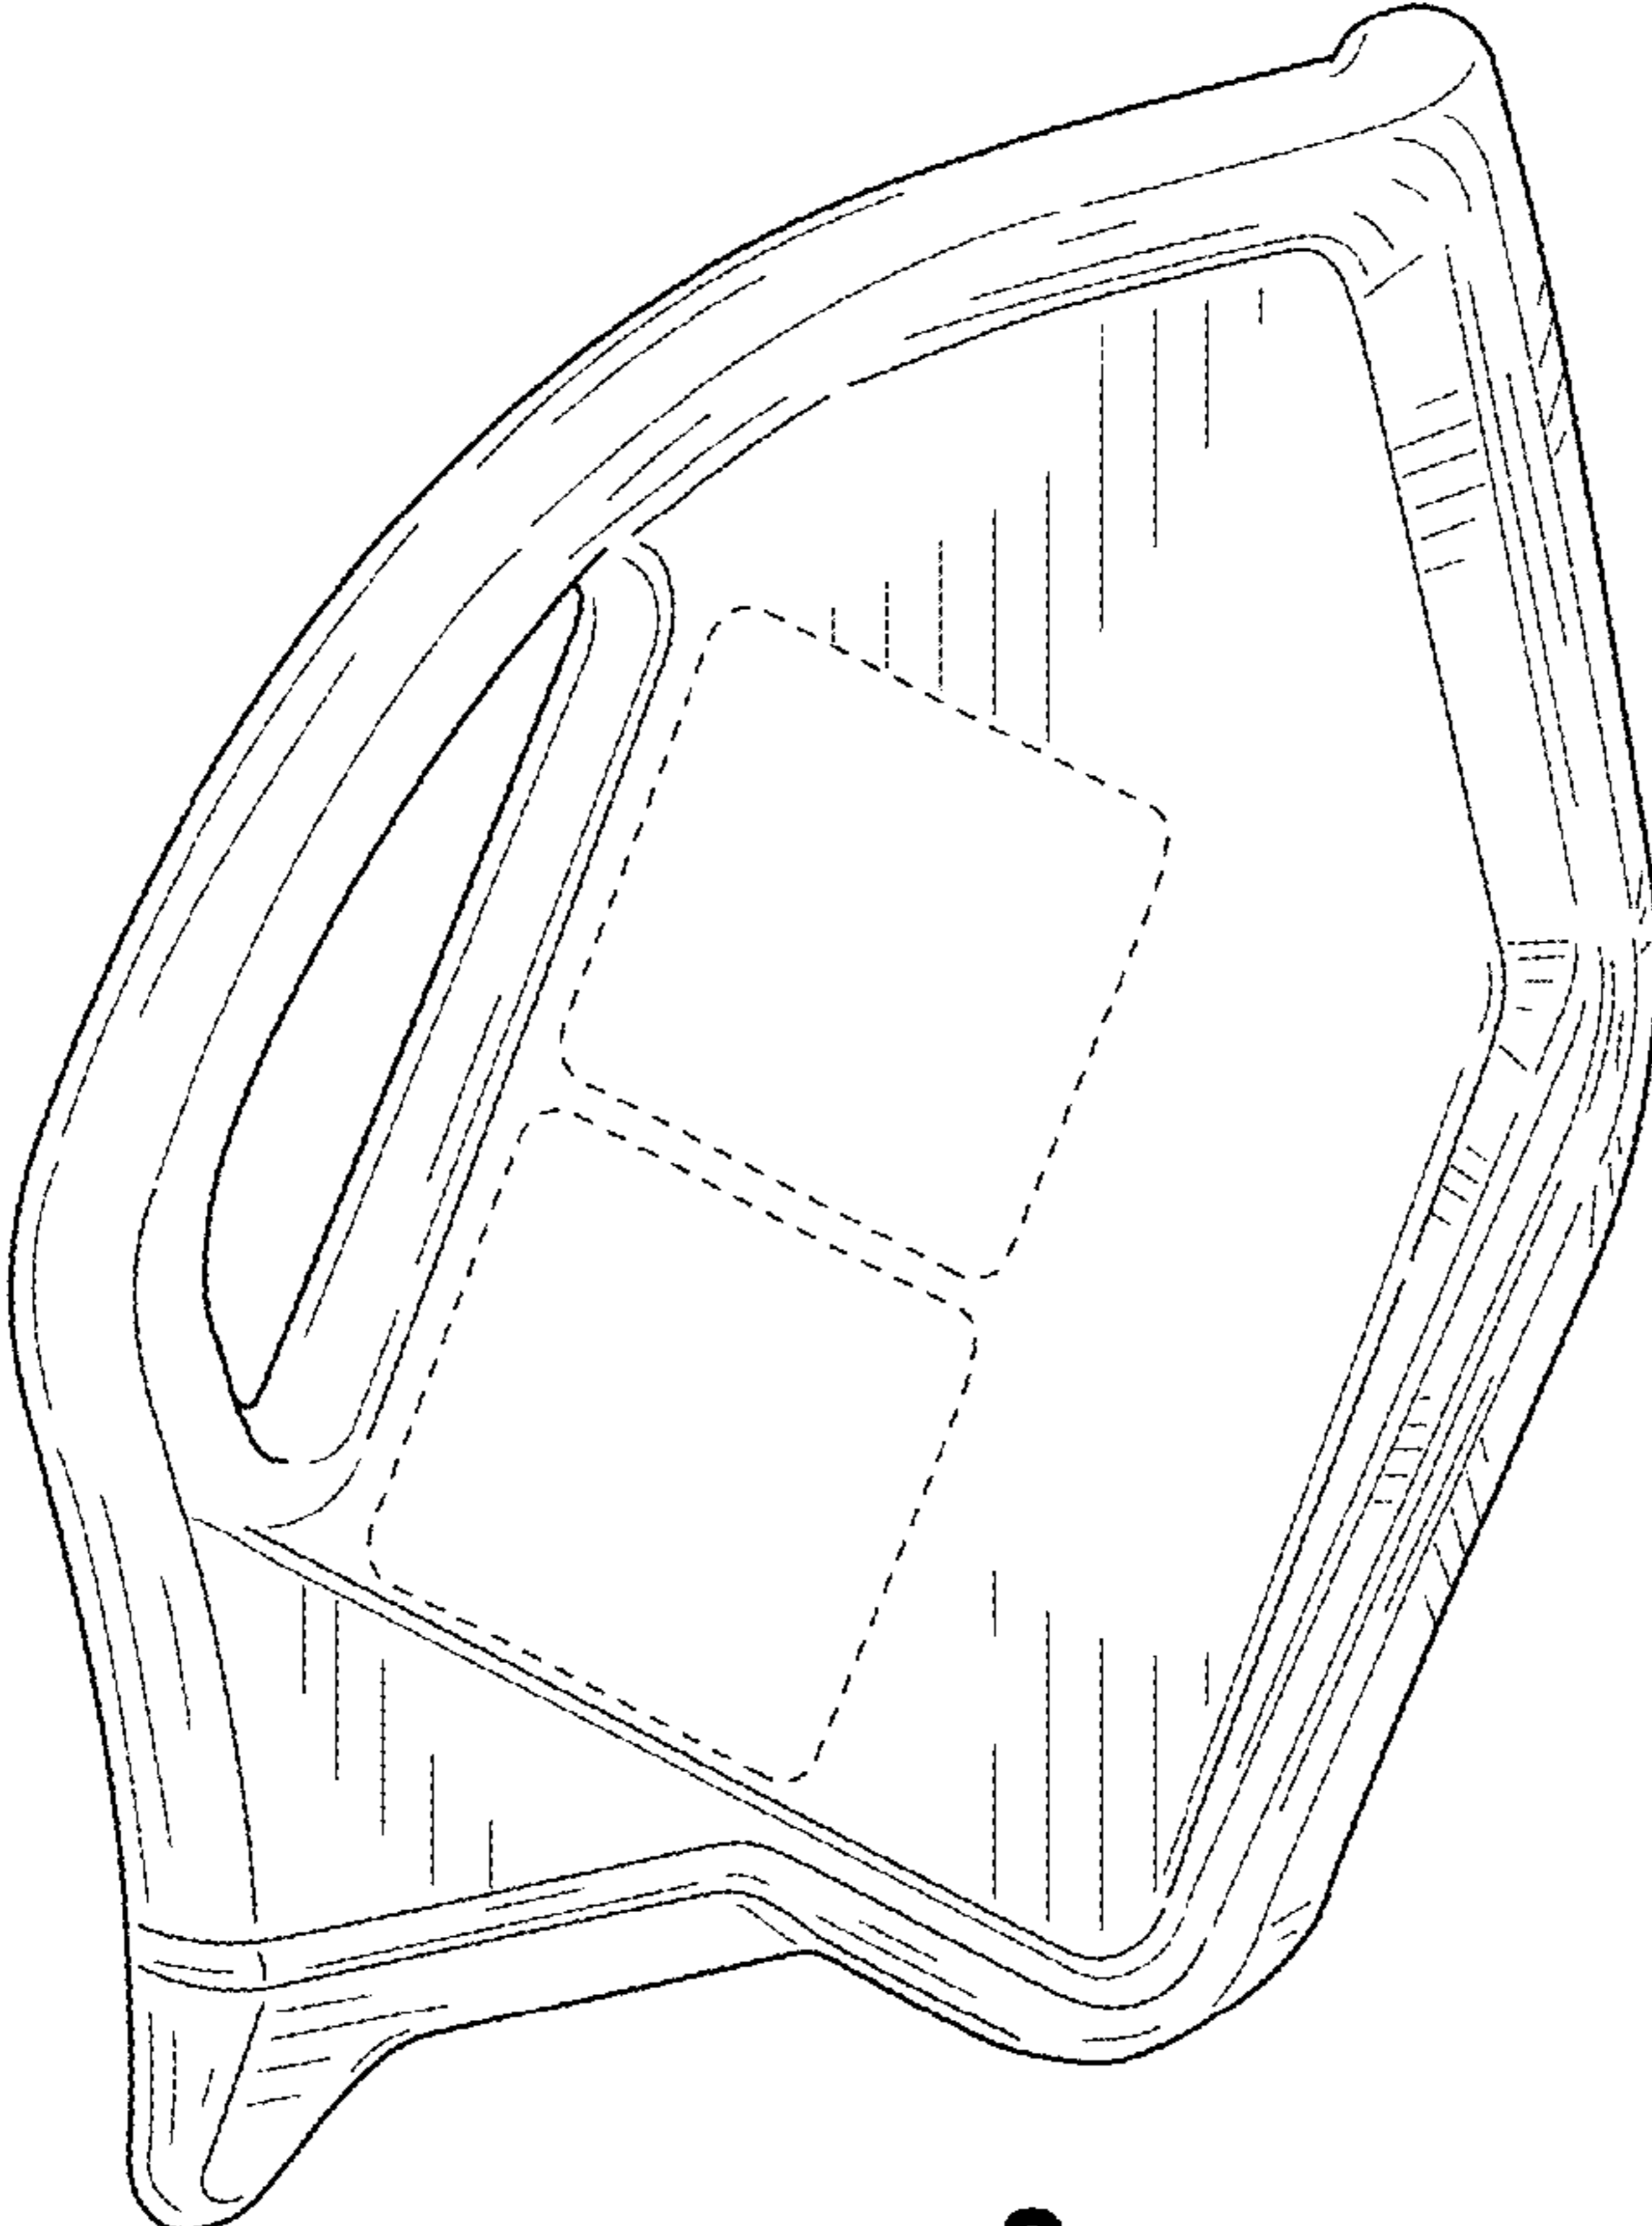


FIG. 2

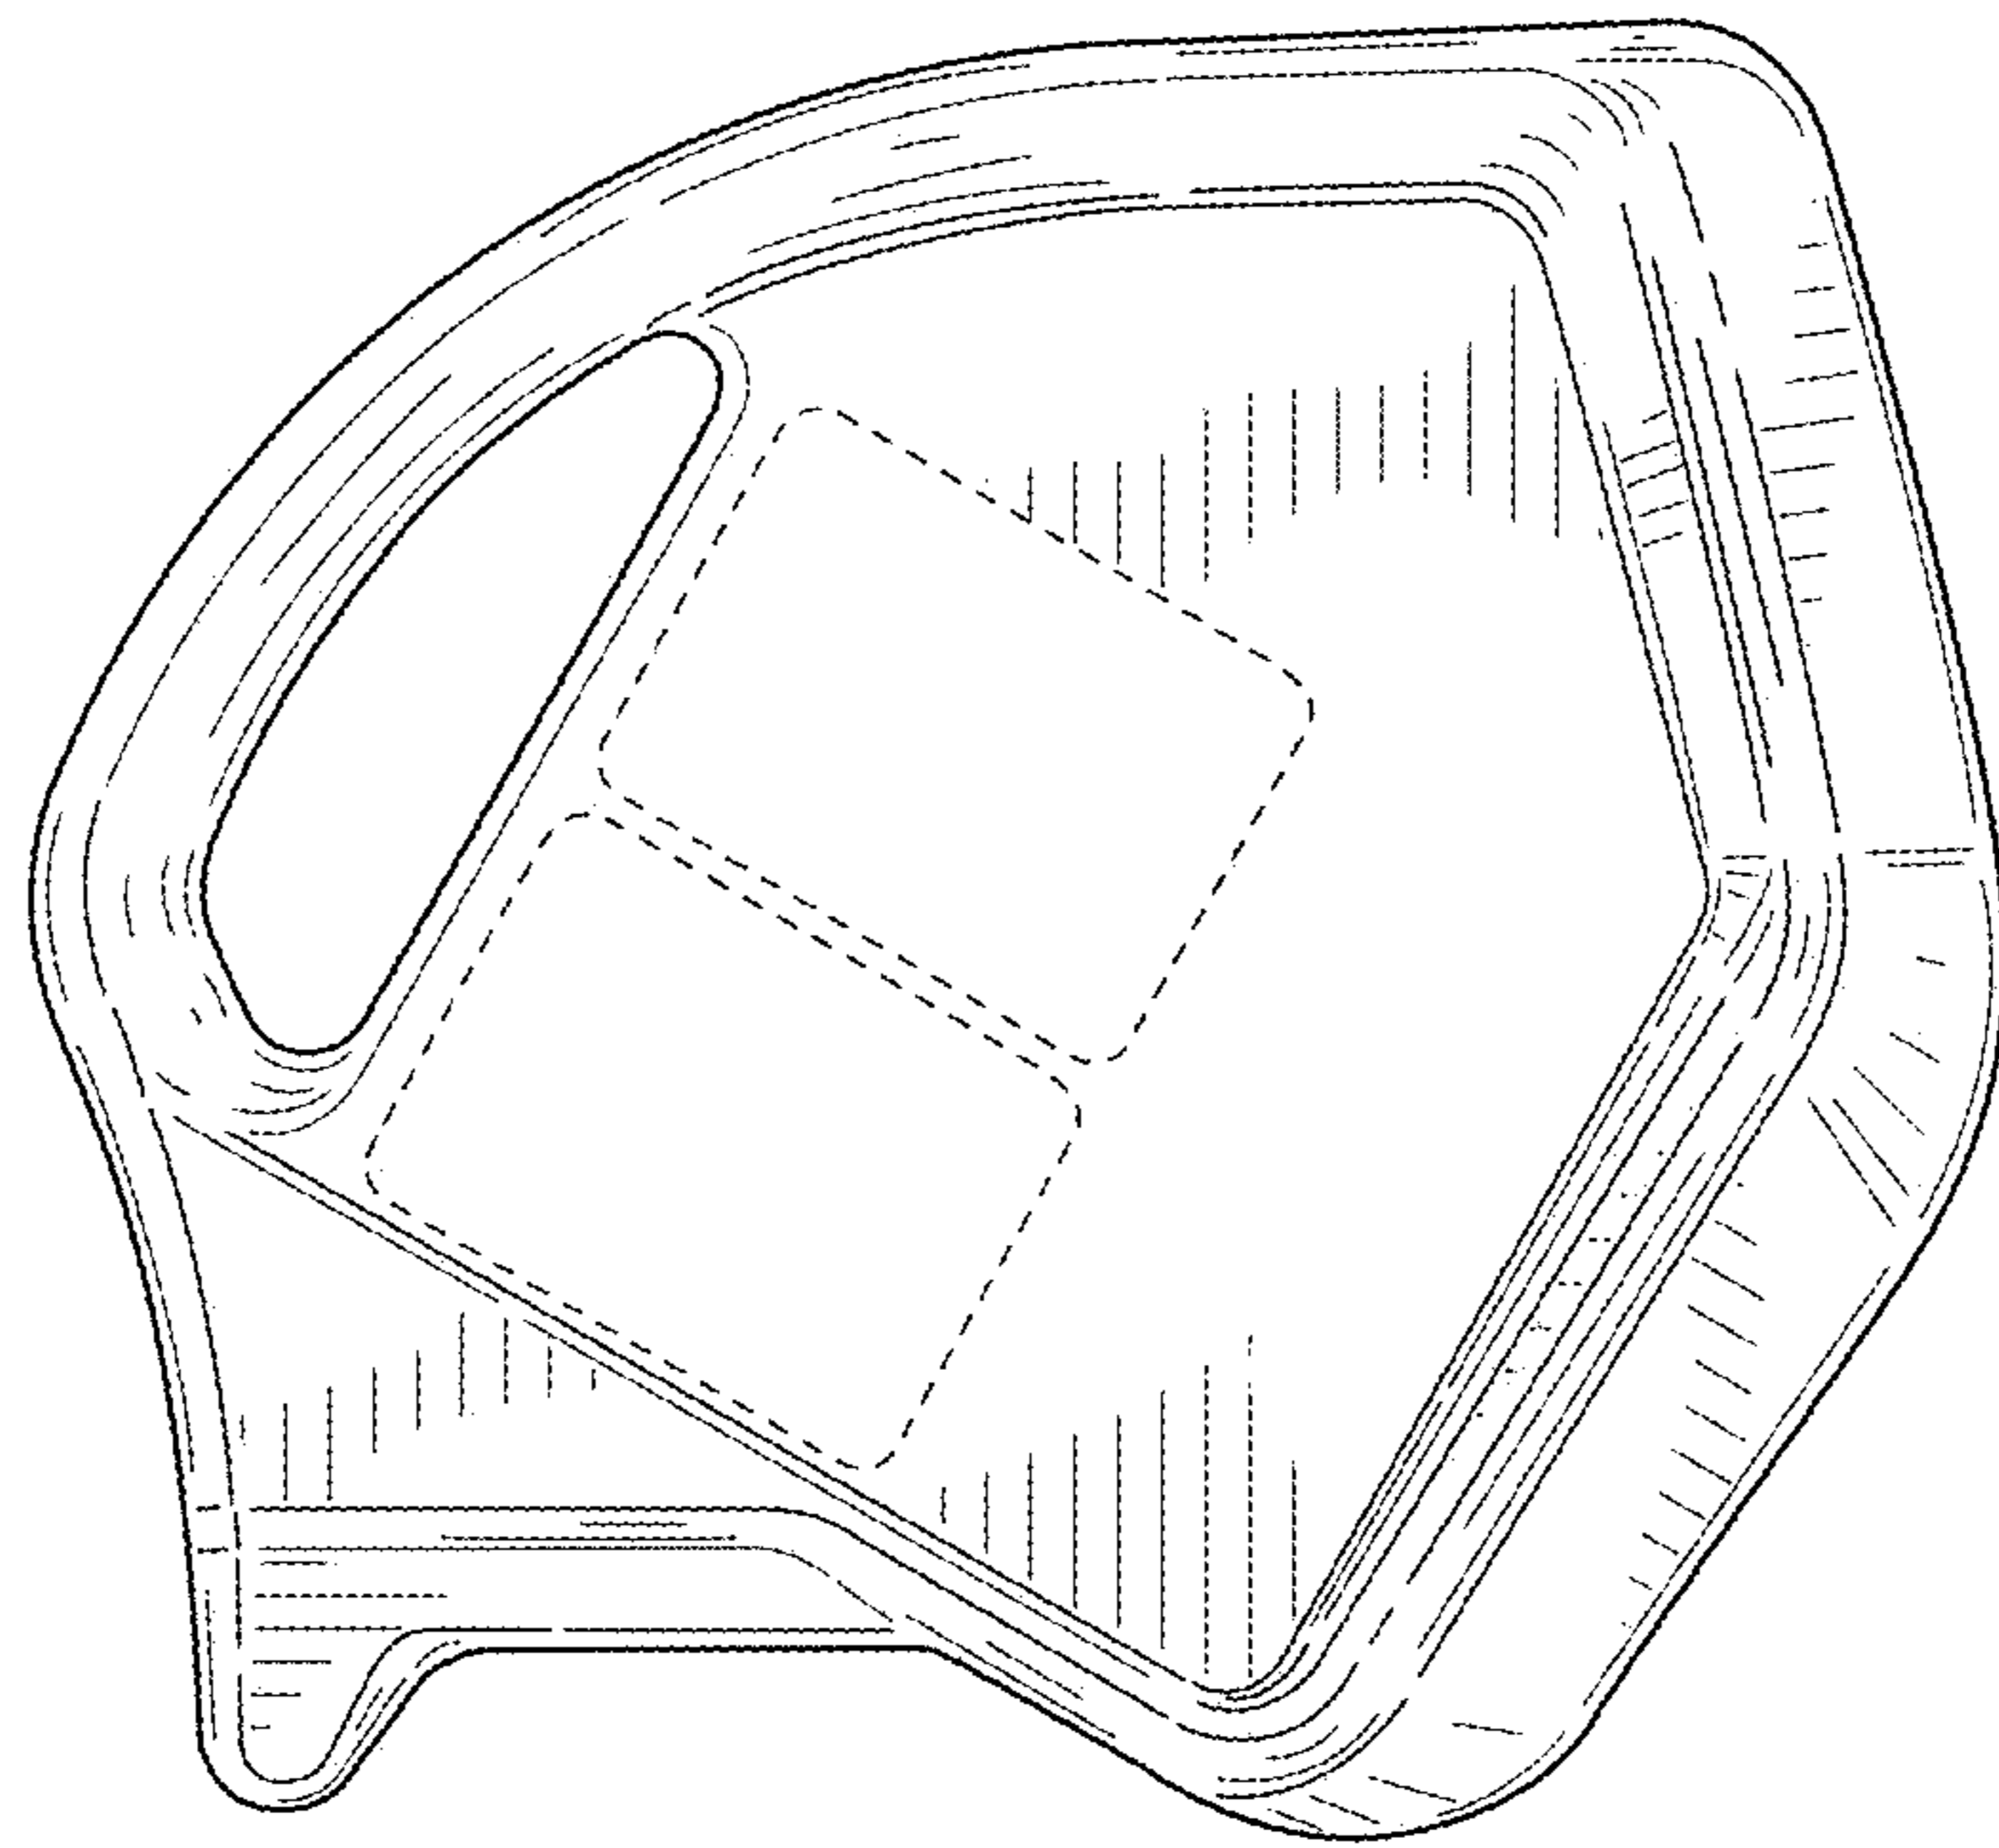


FIG. 3

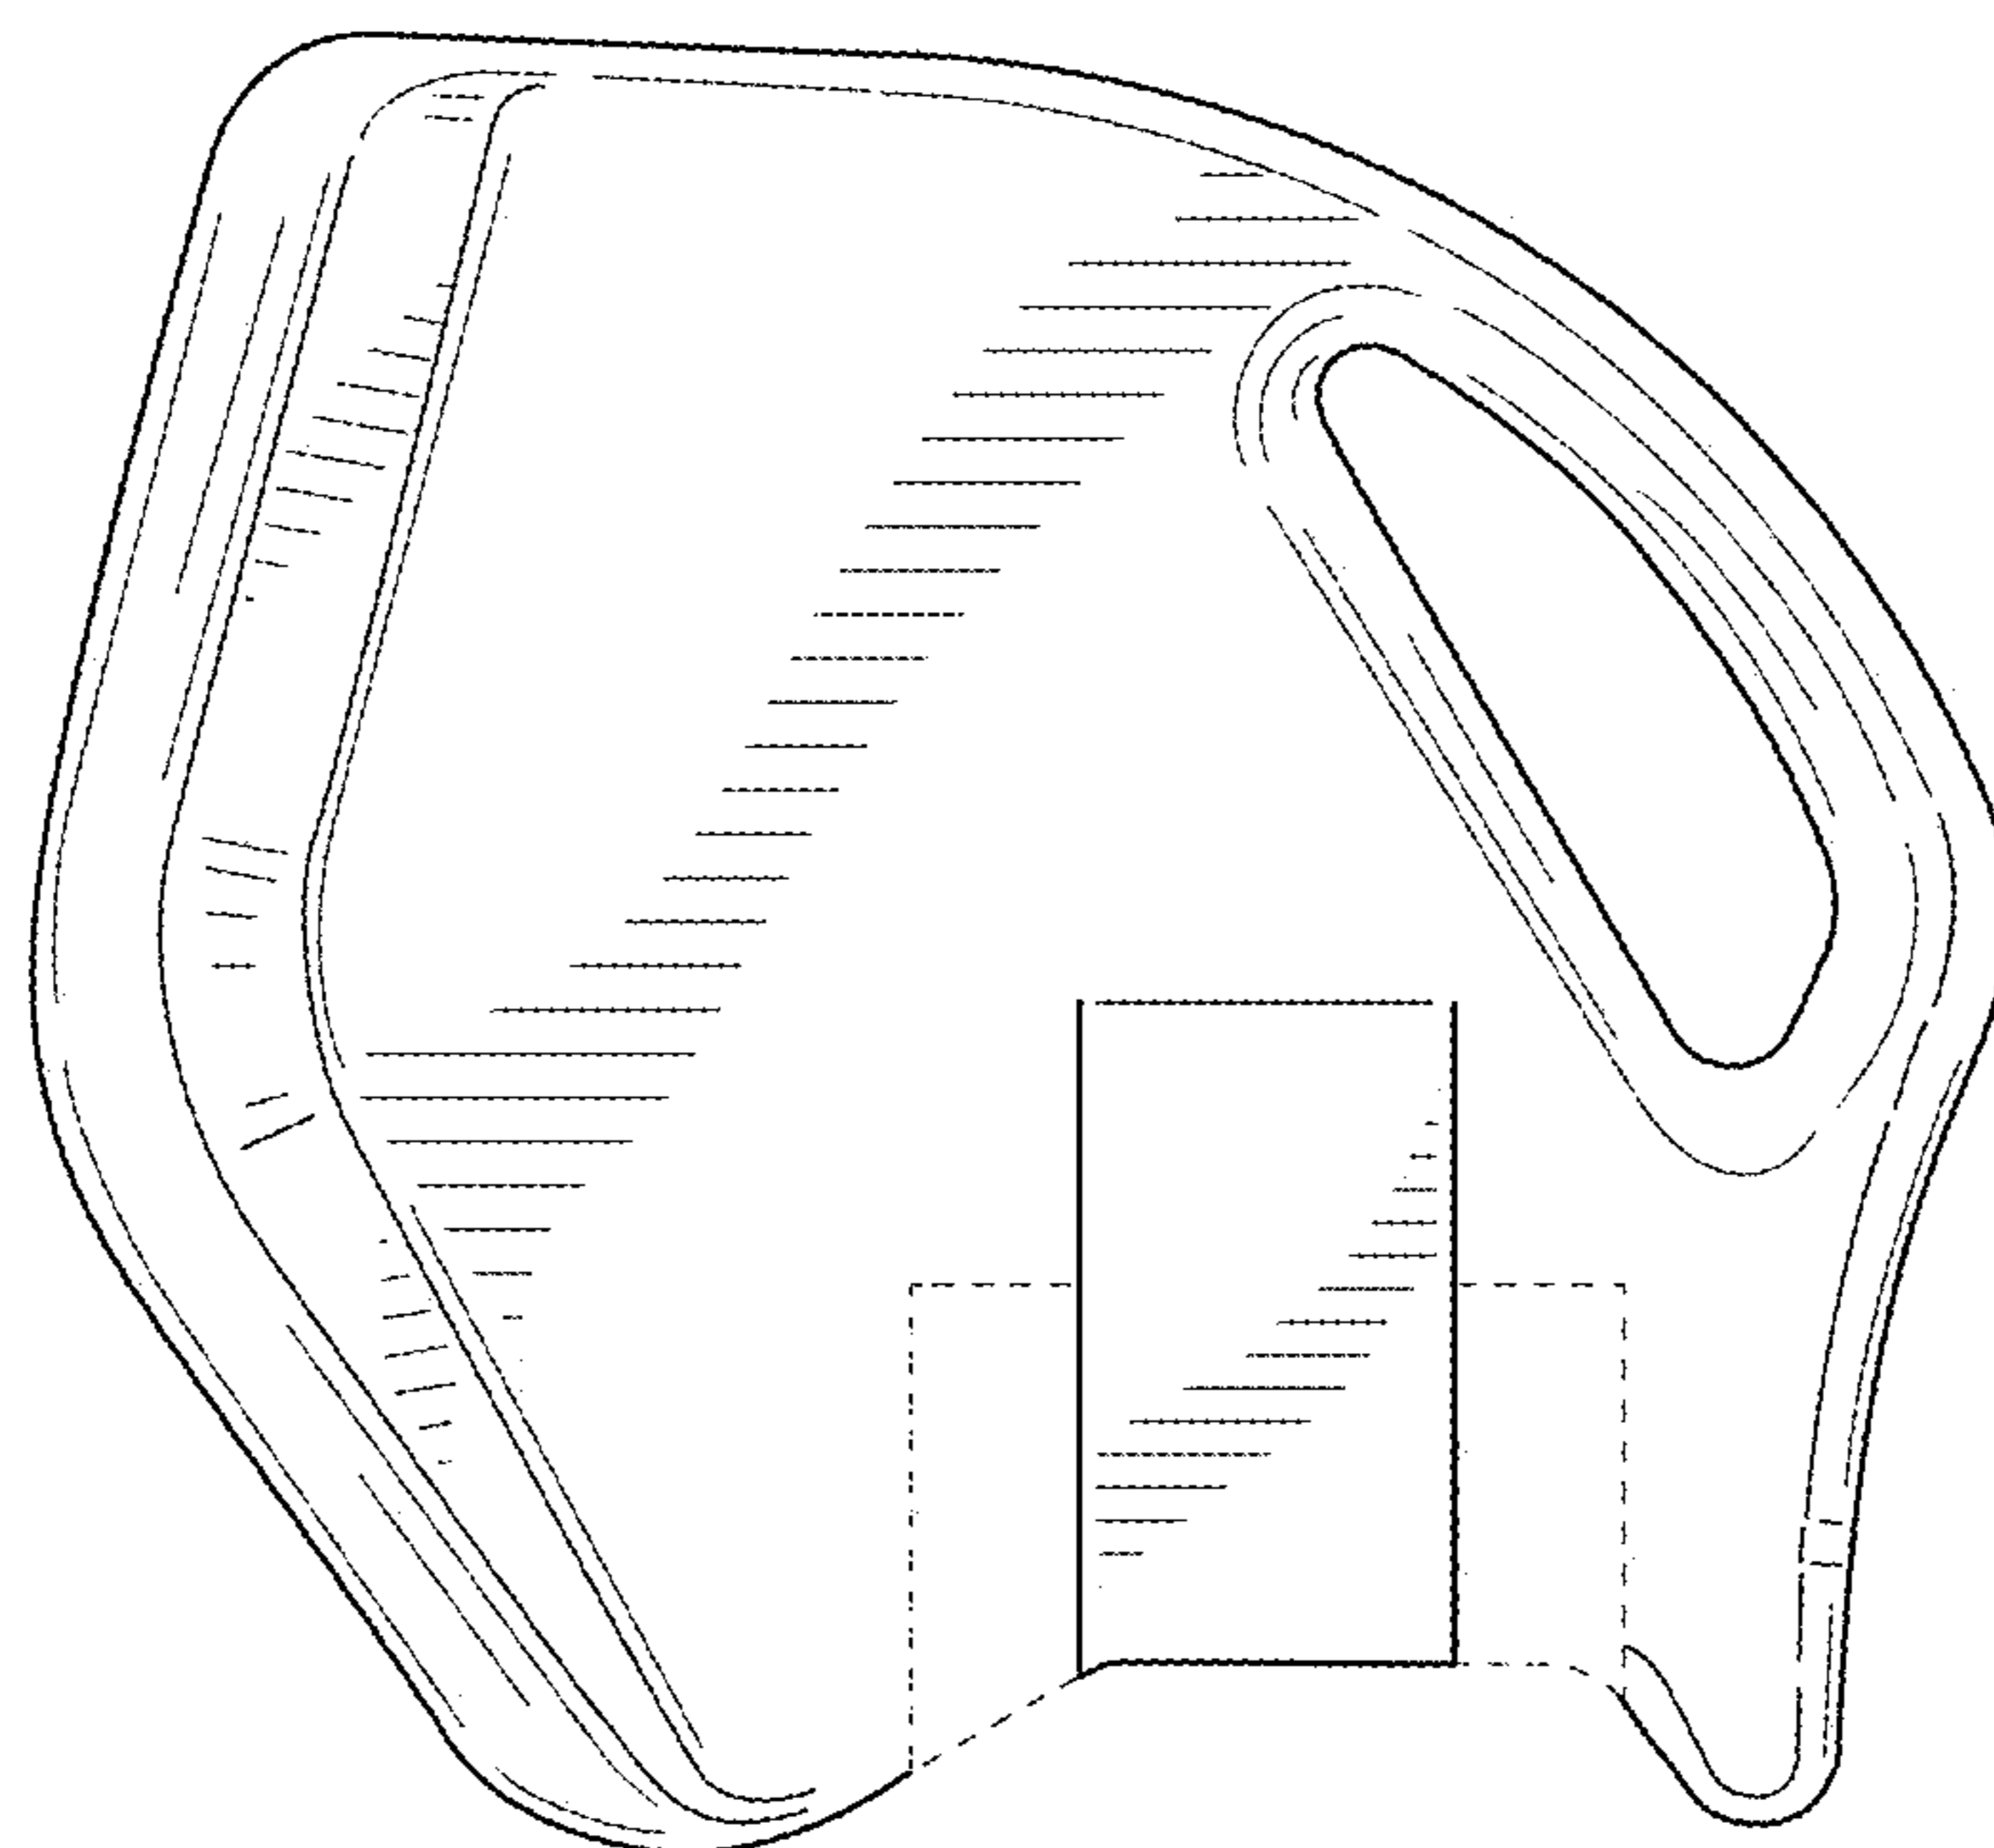


FIG. 4

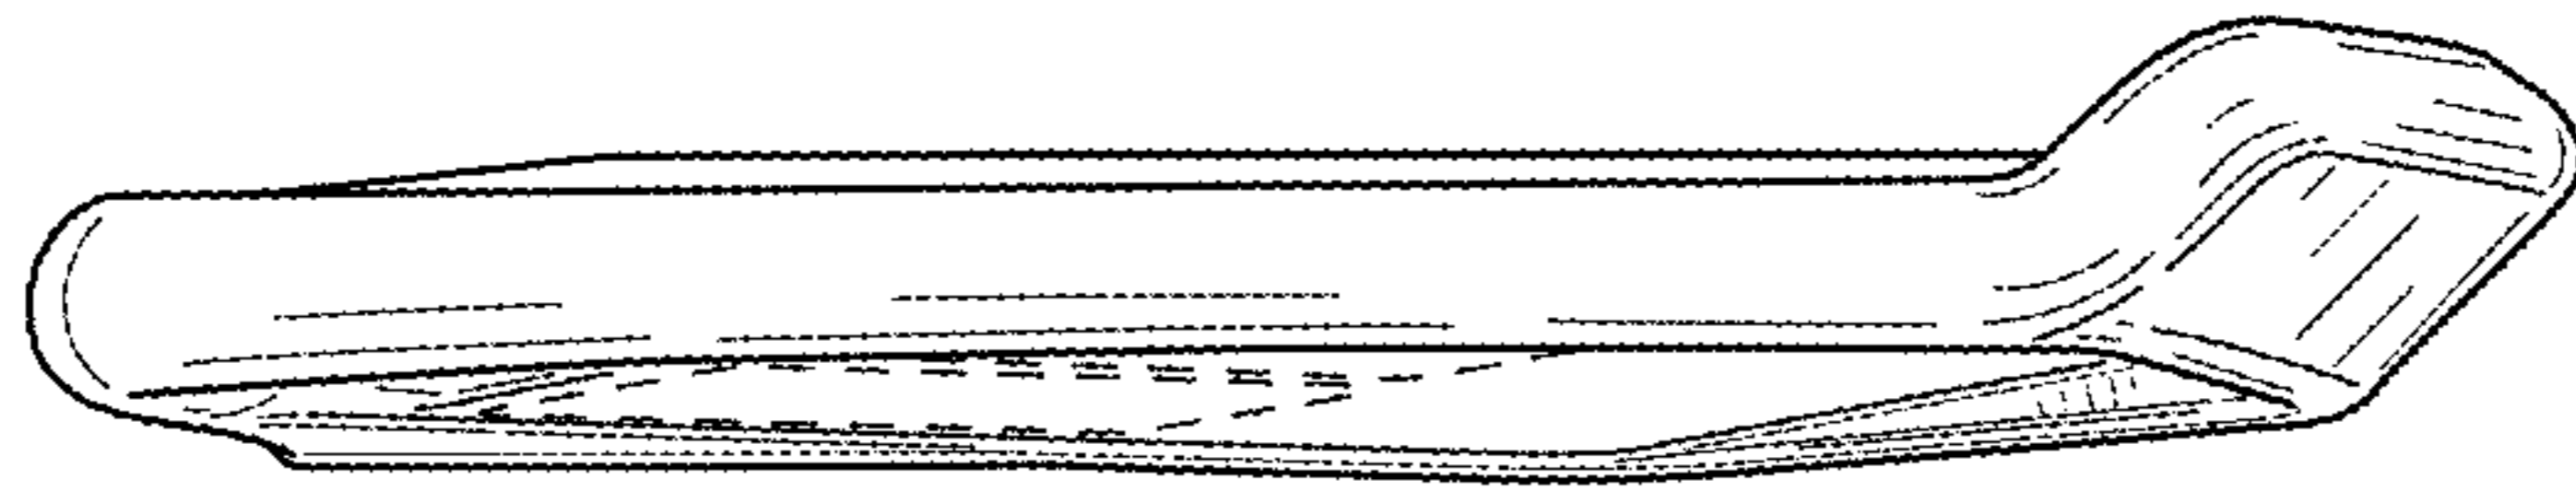


FIG. 5

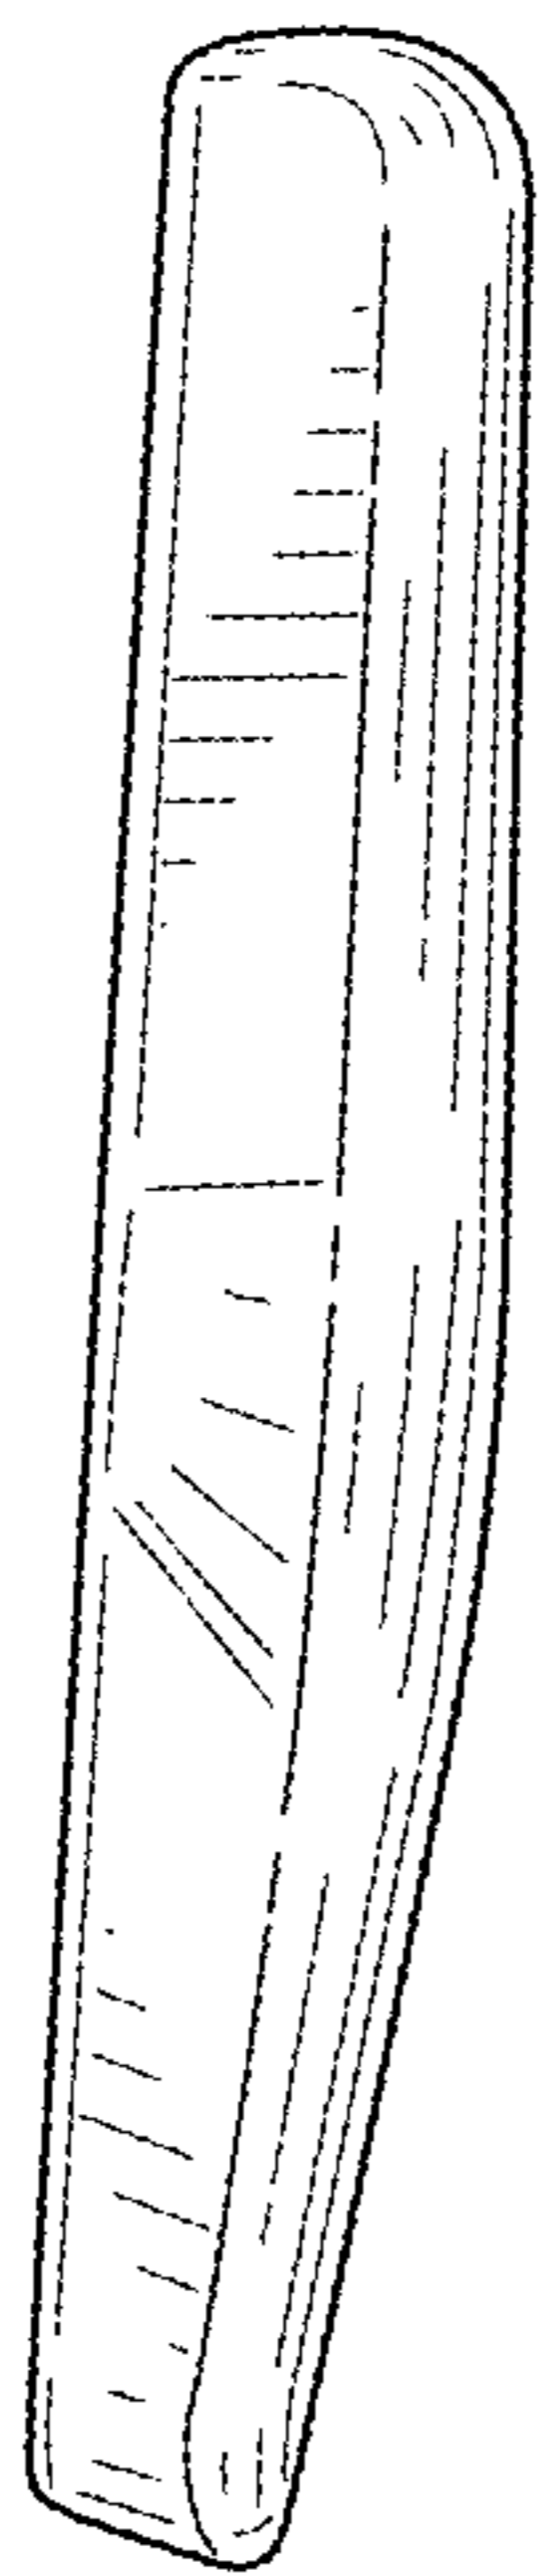


FIG. 6

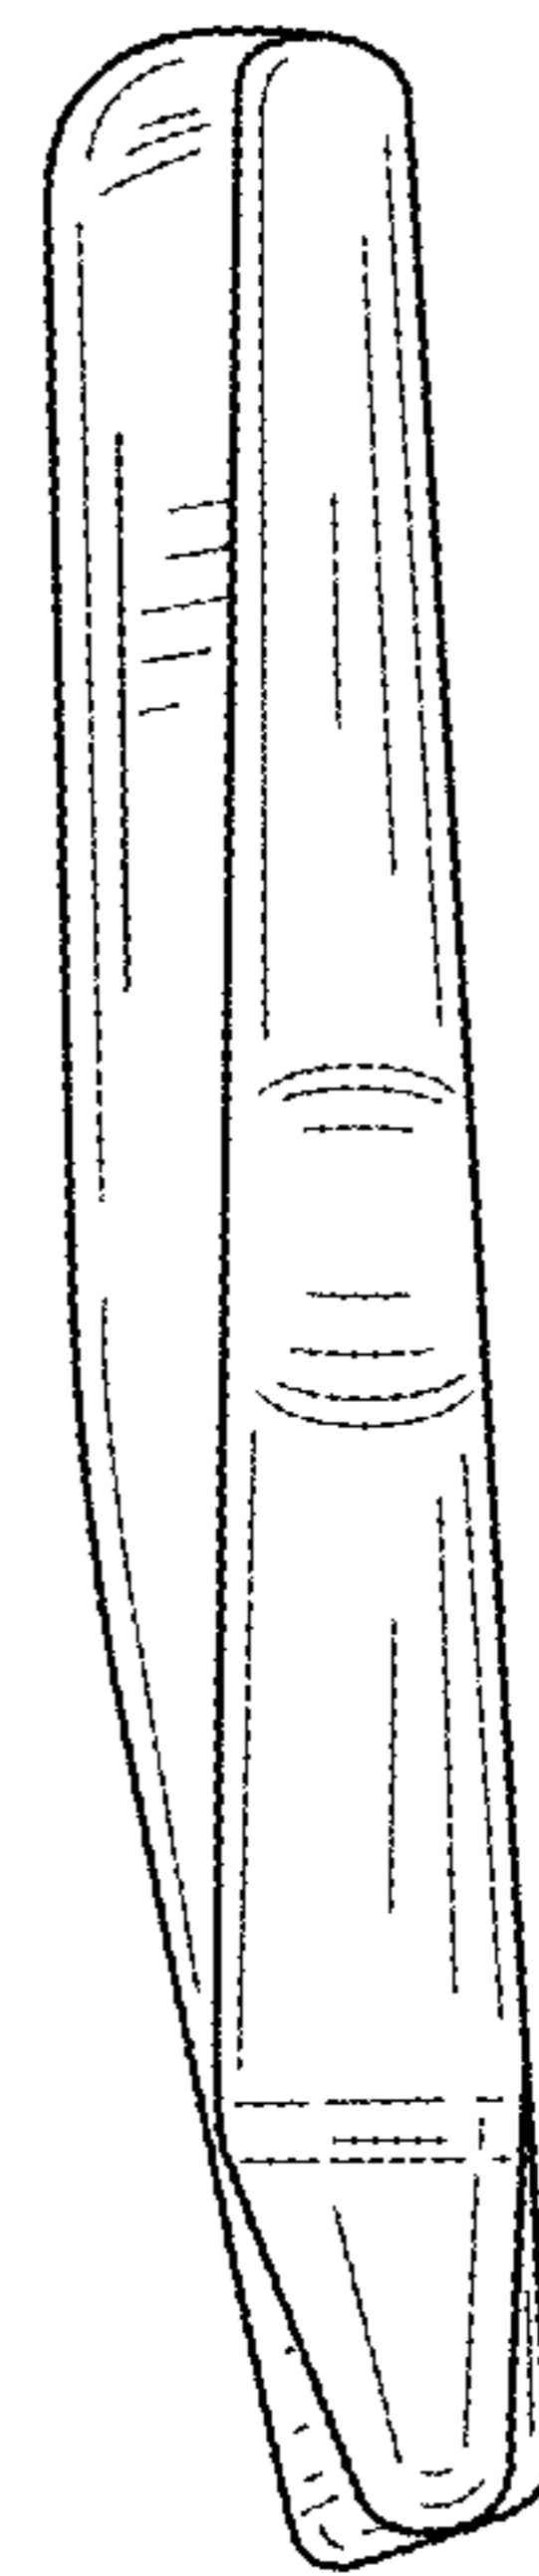


FIG. 7

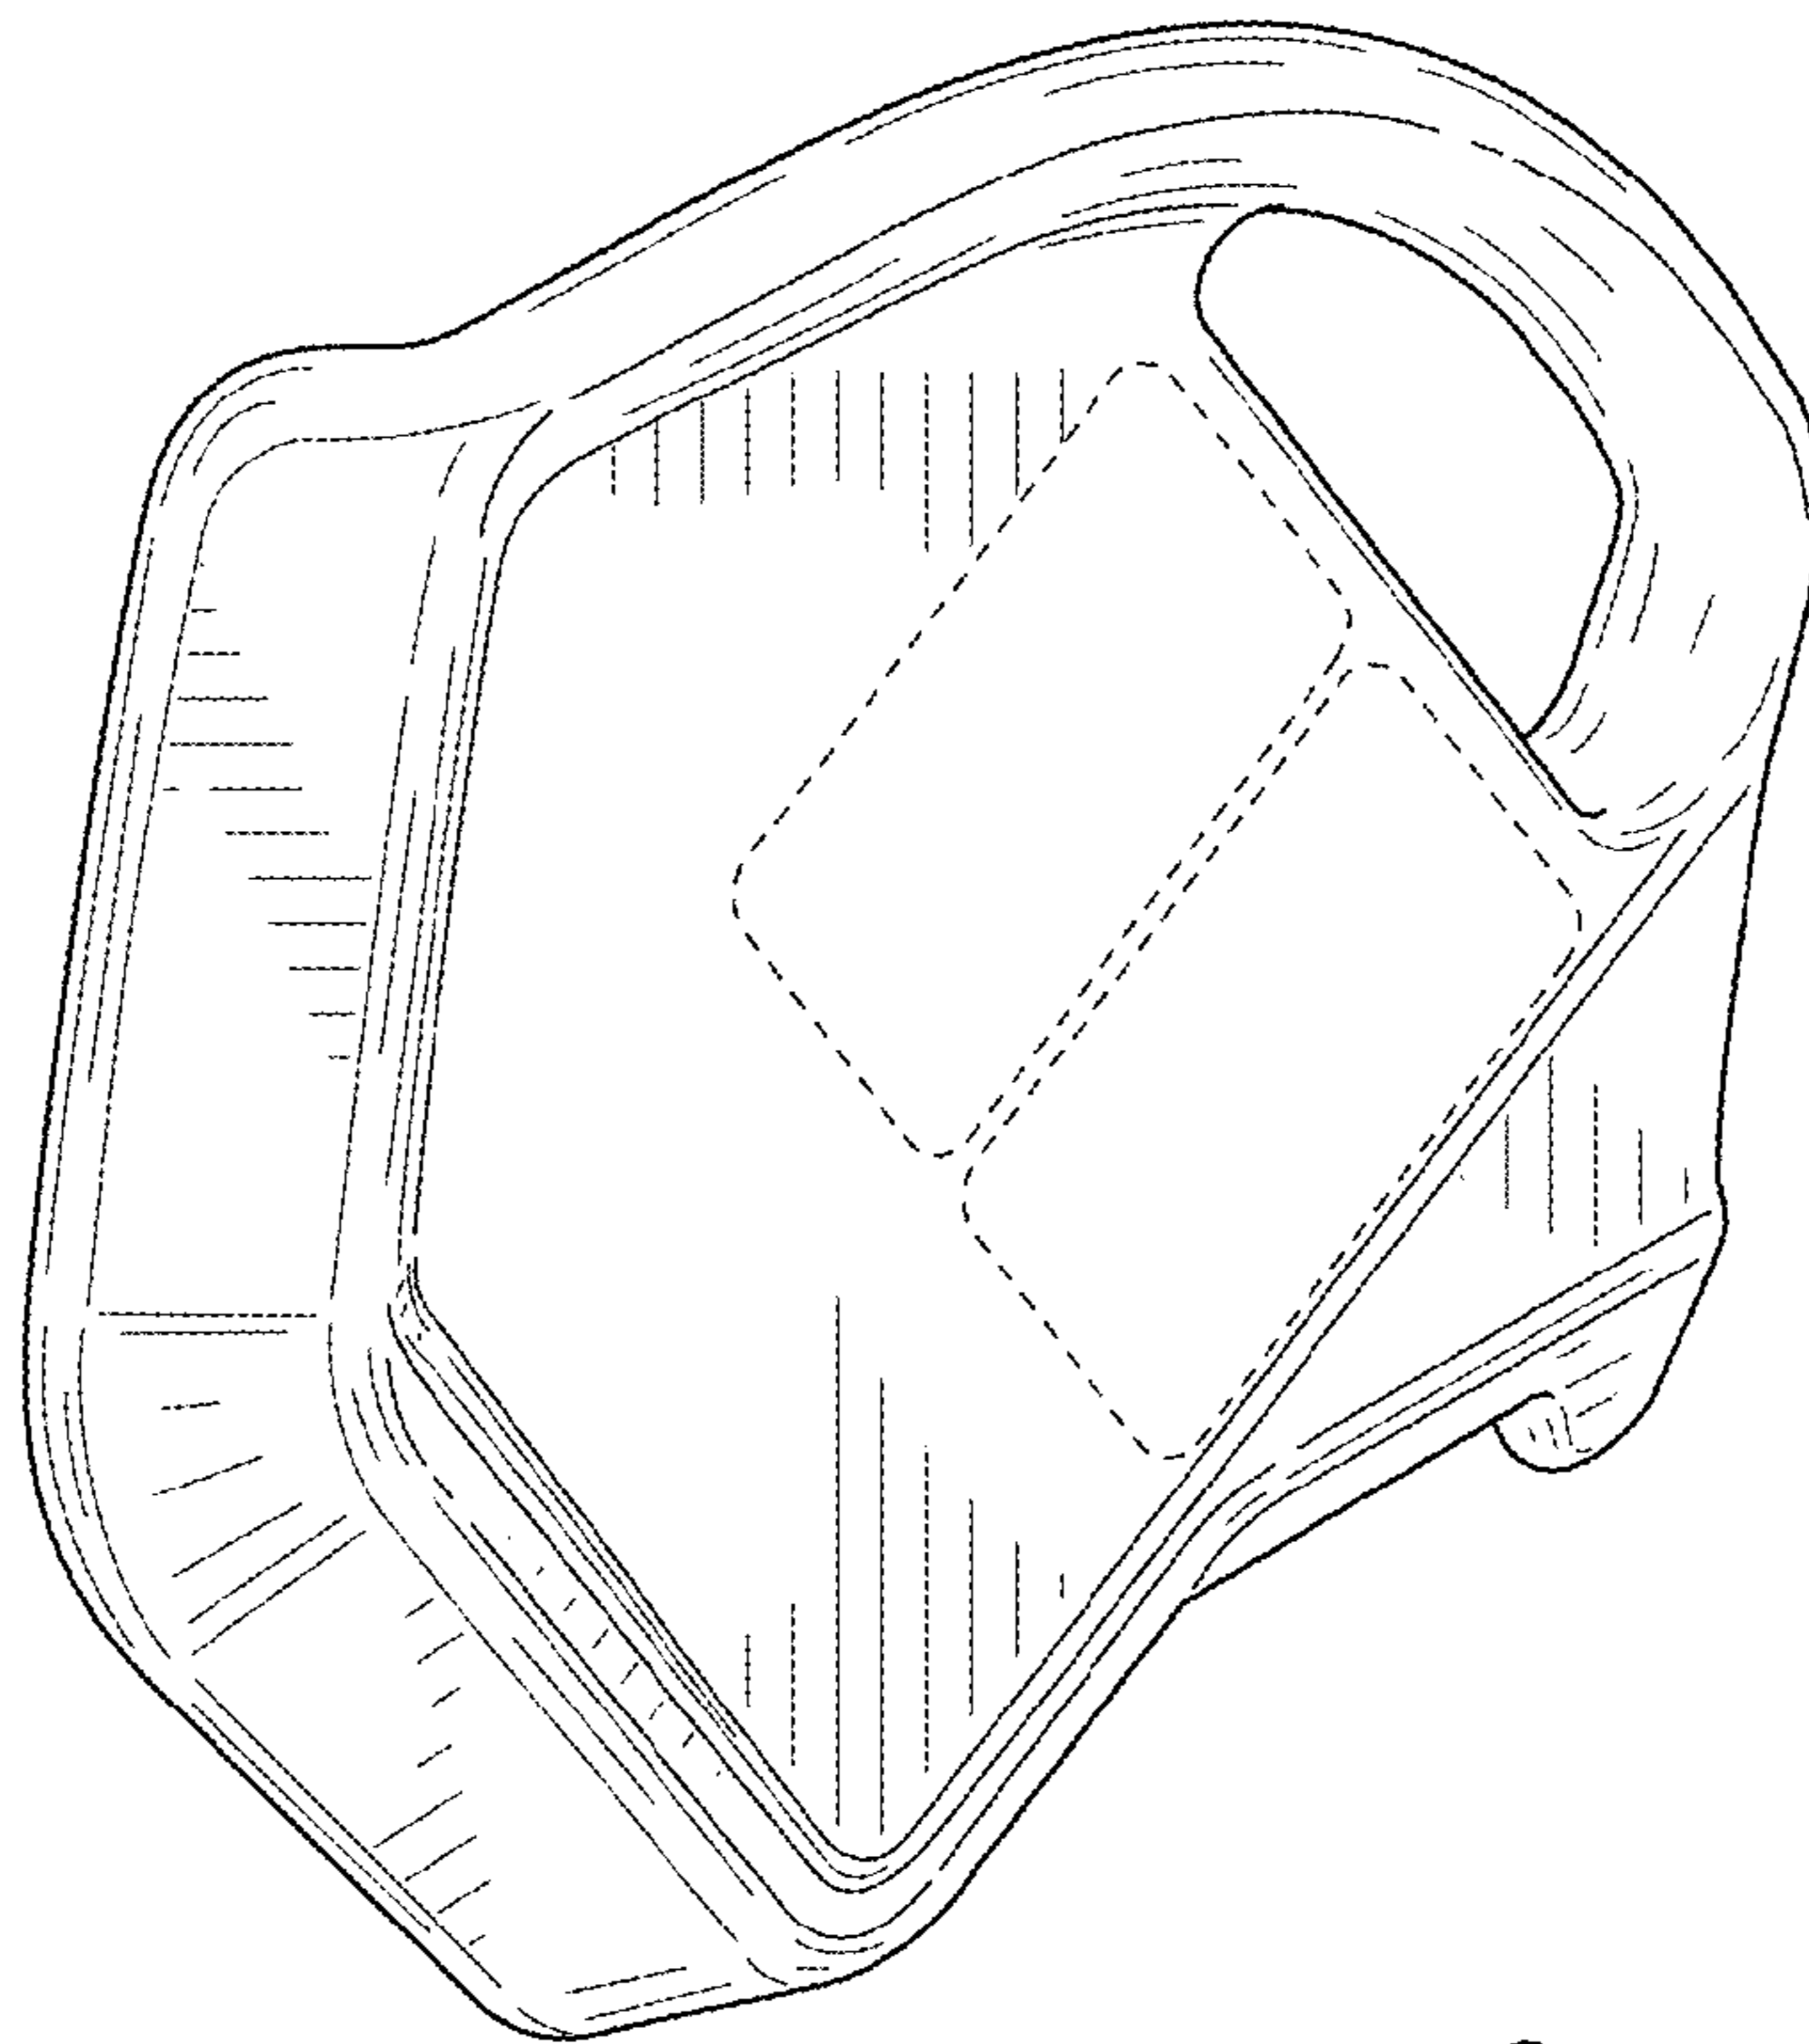


FIG. 8

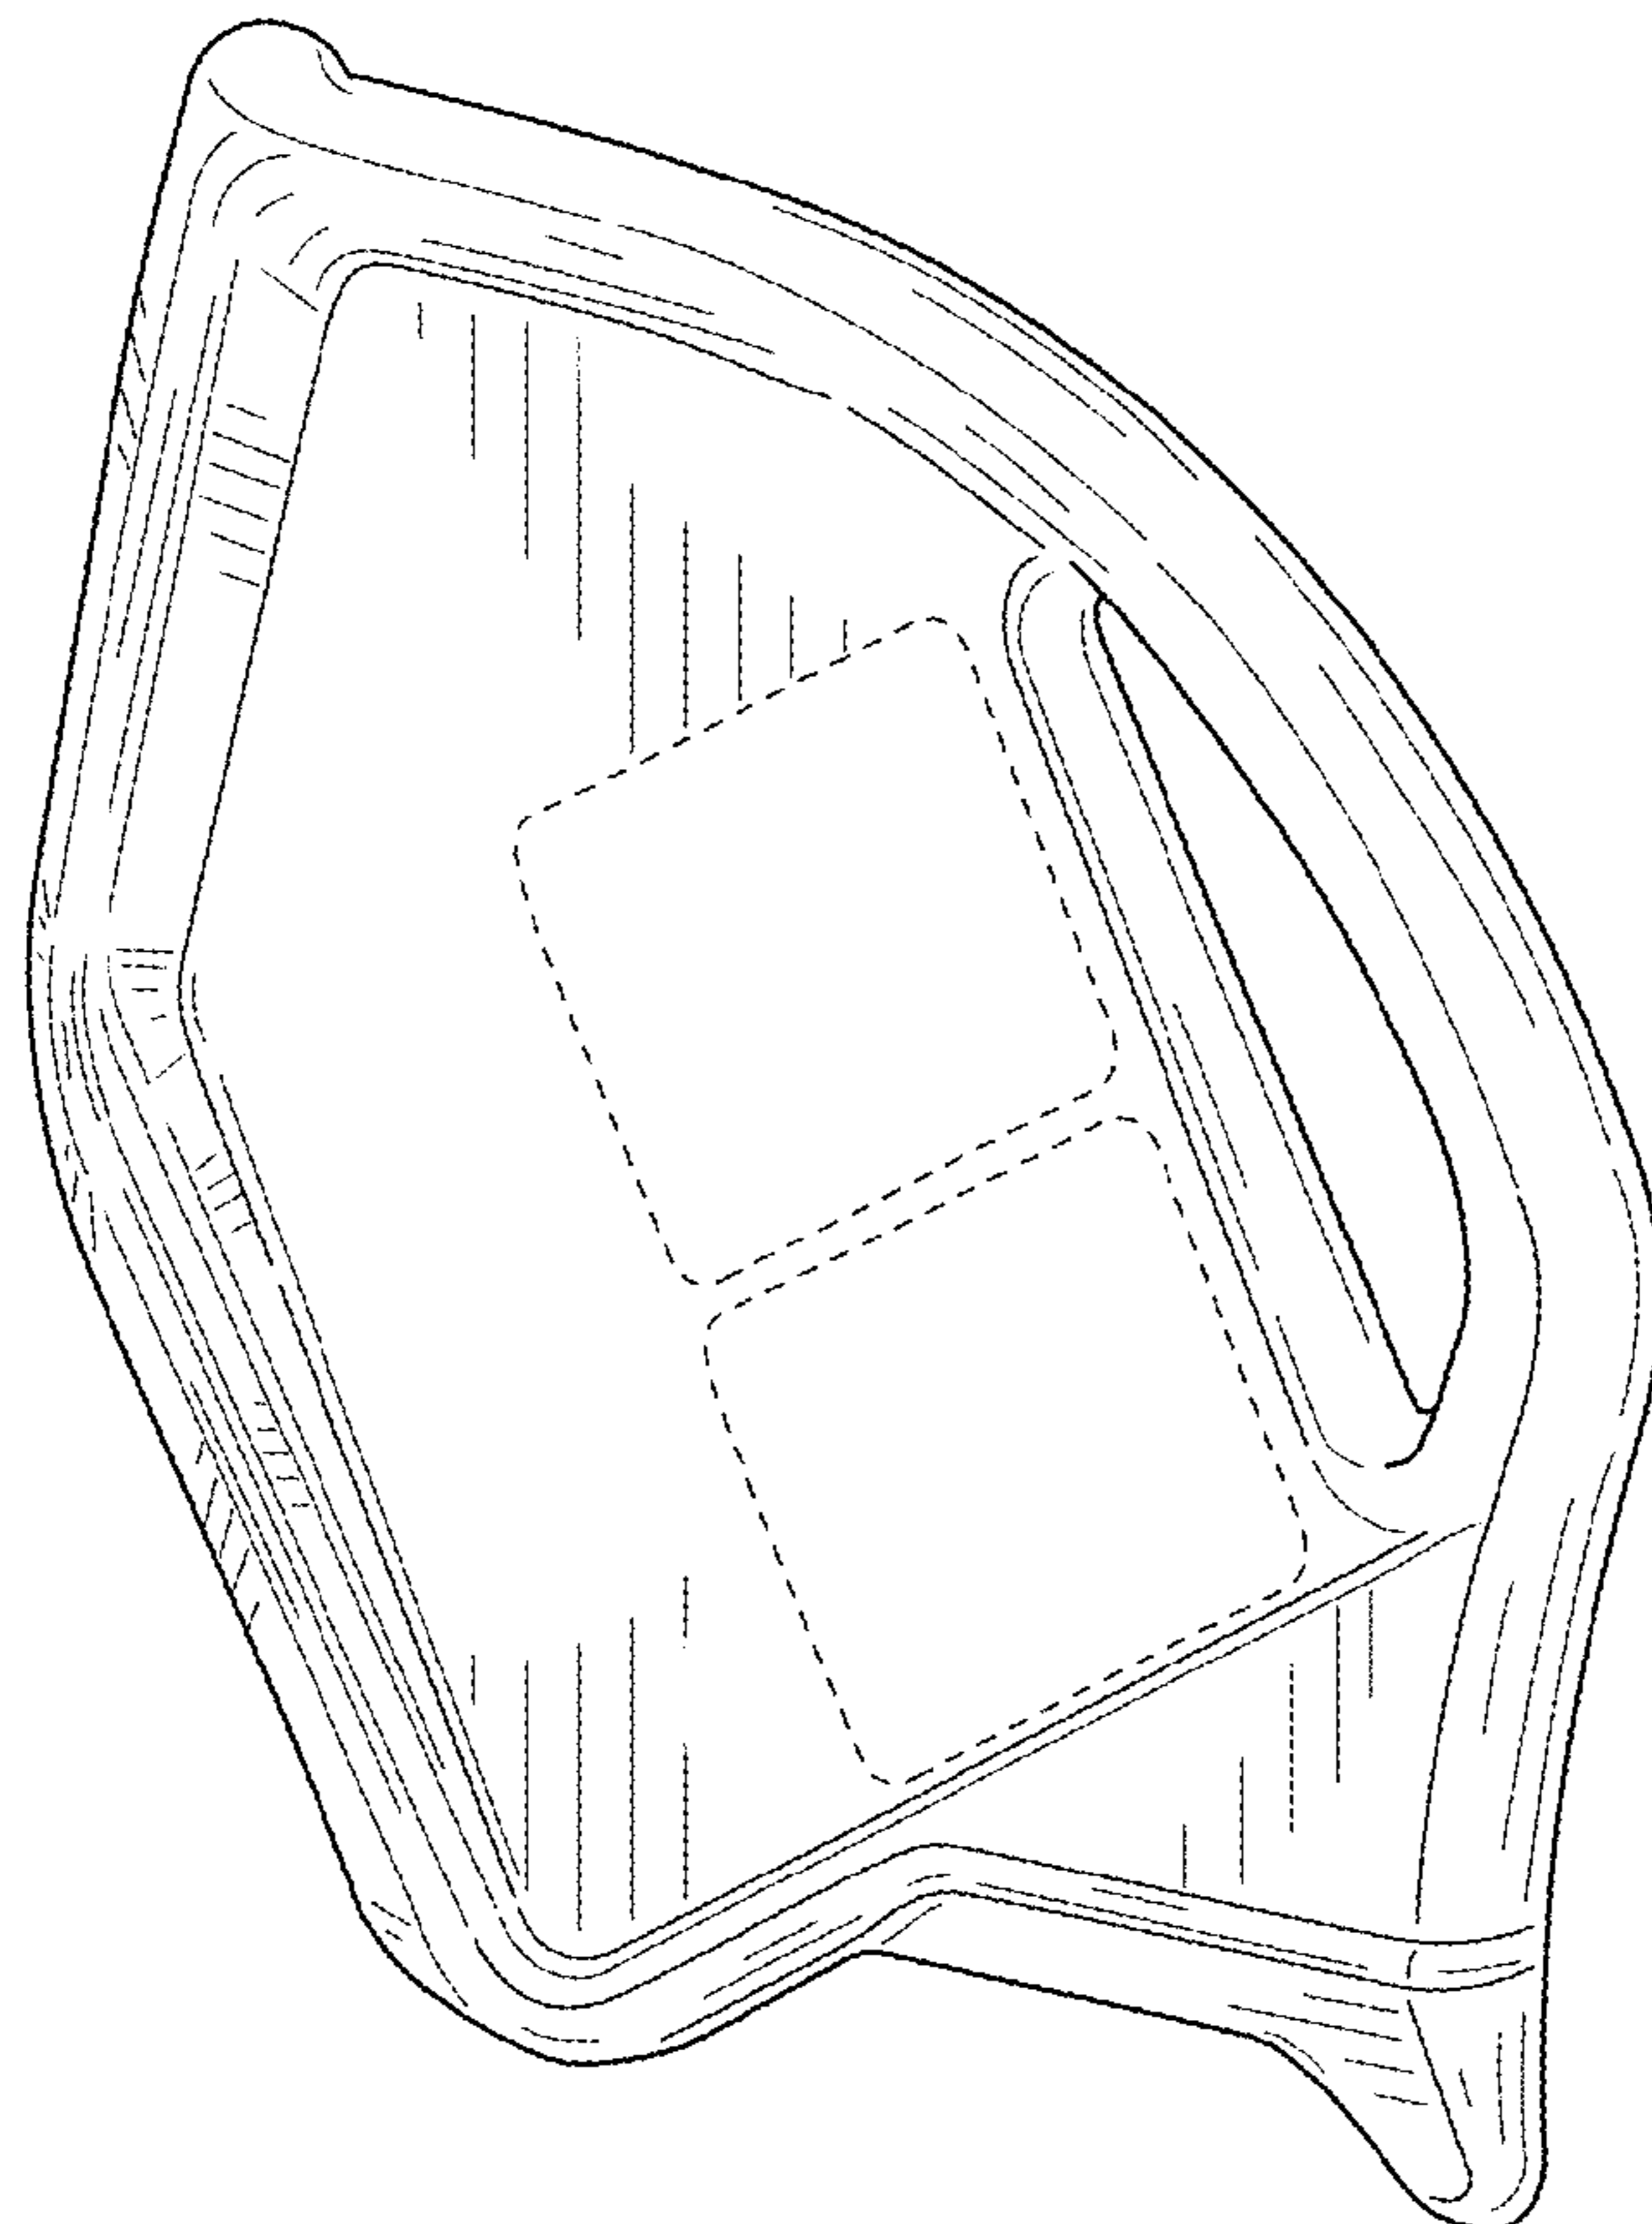


FIG. 9

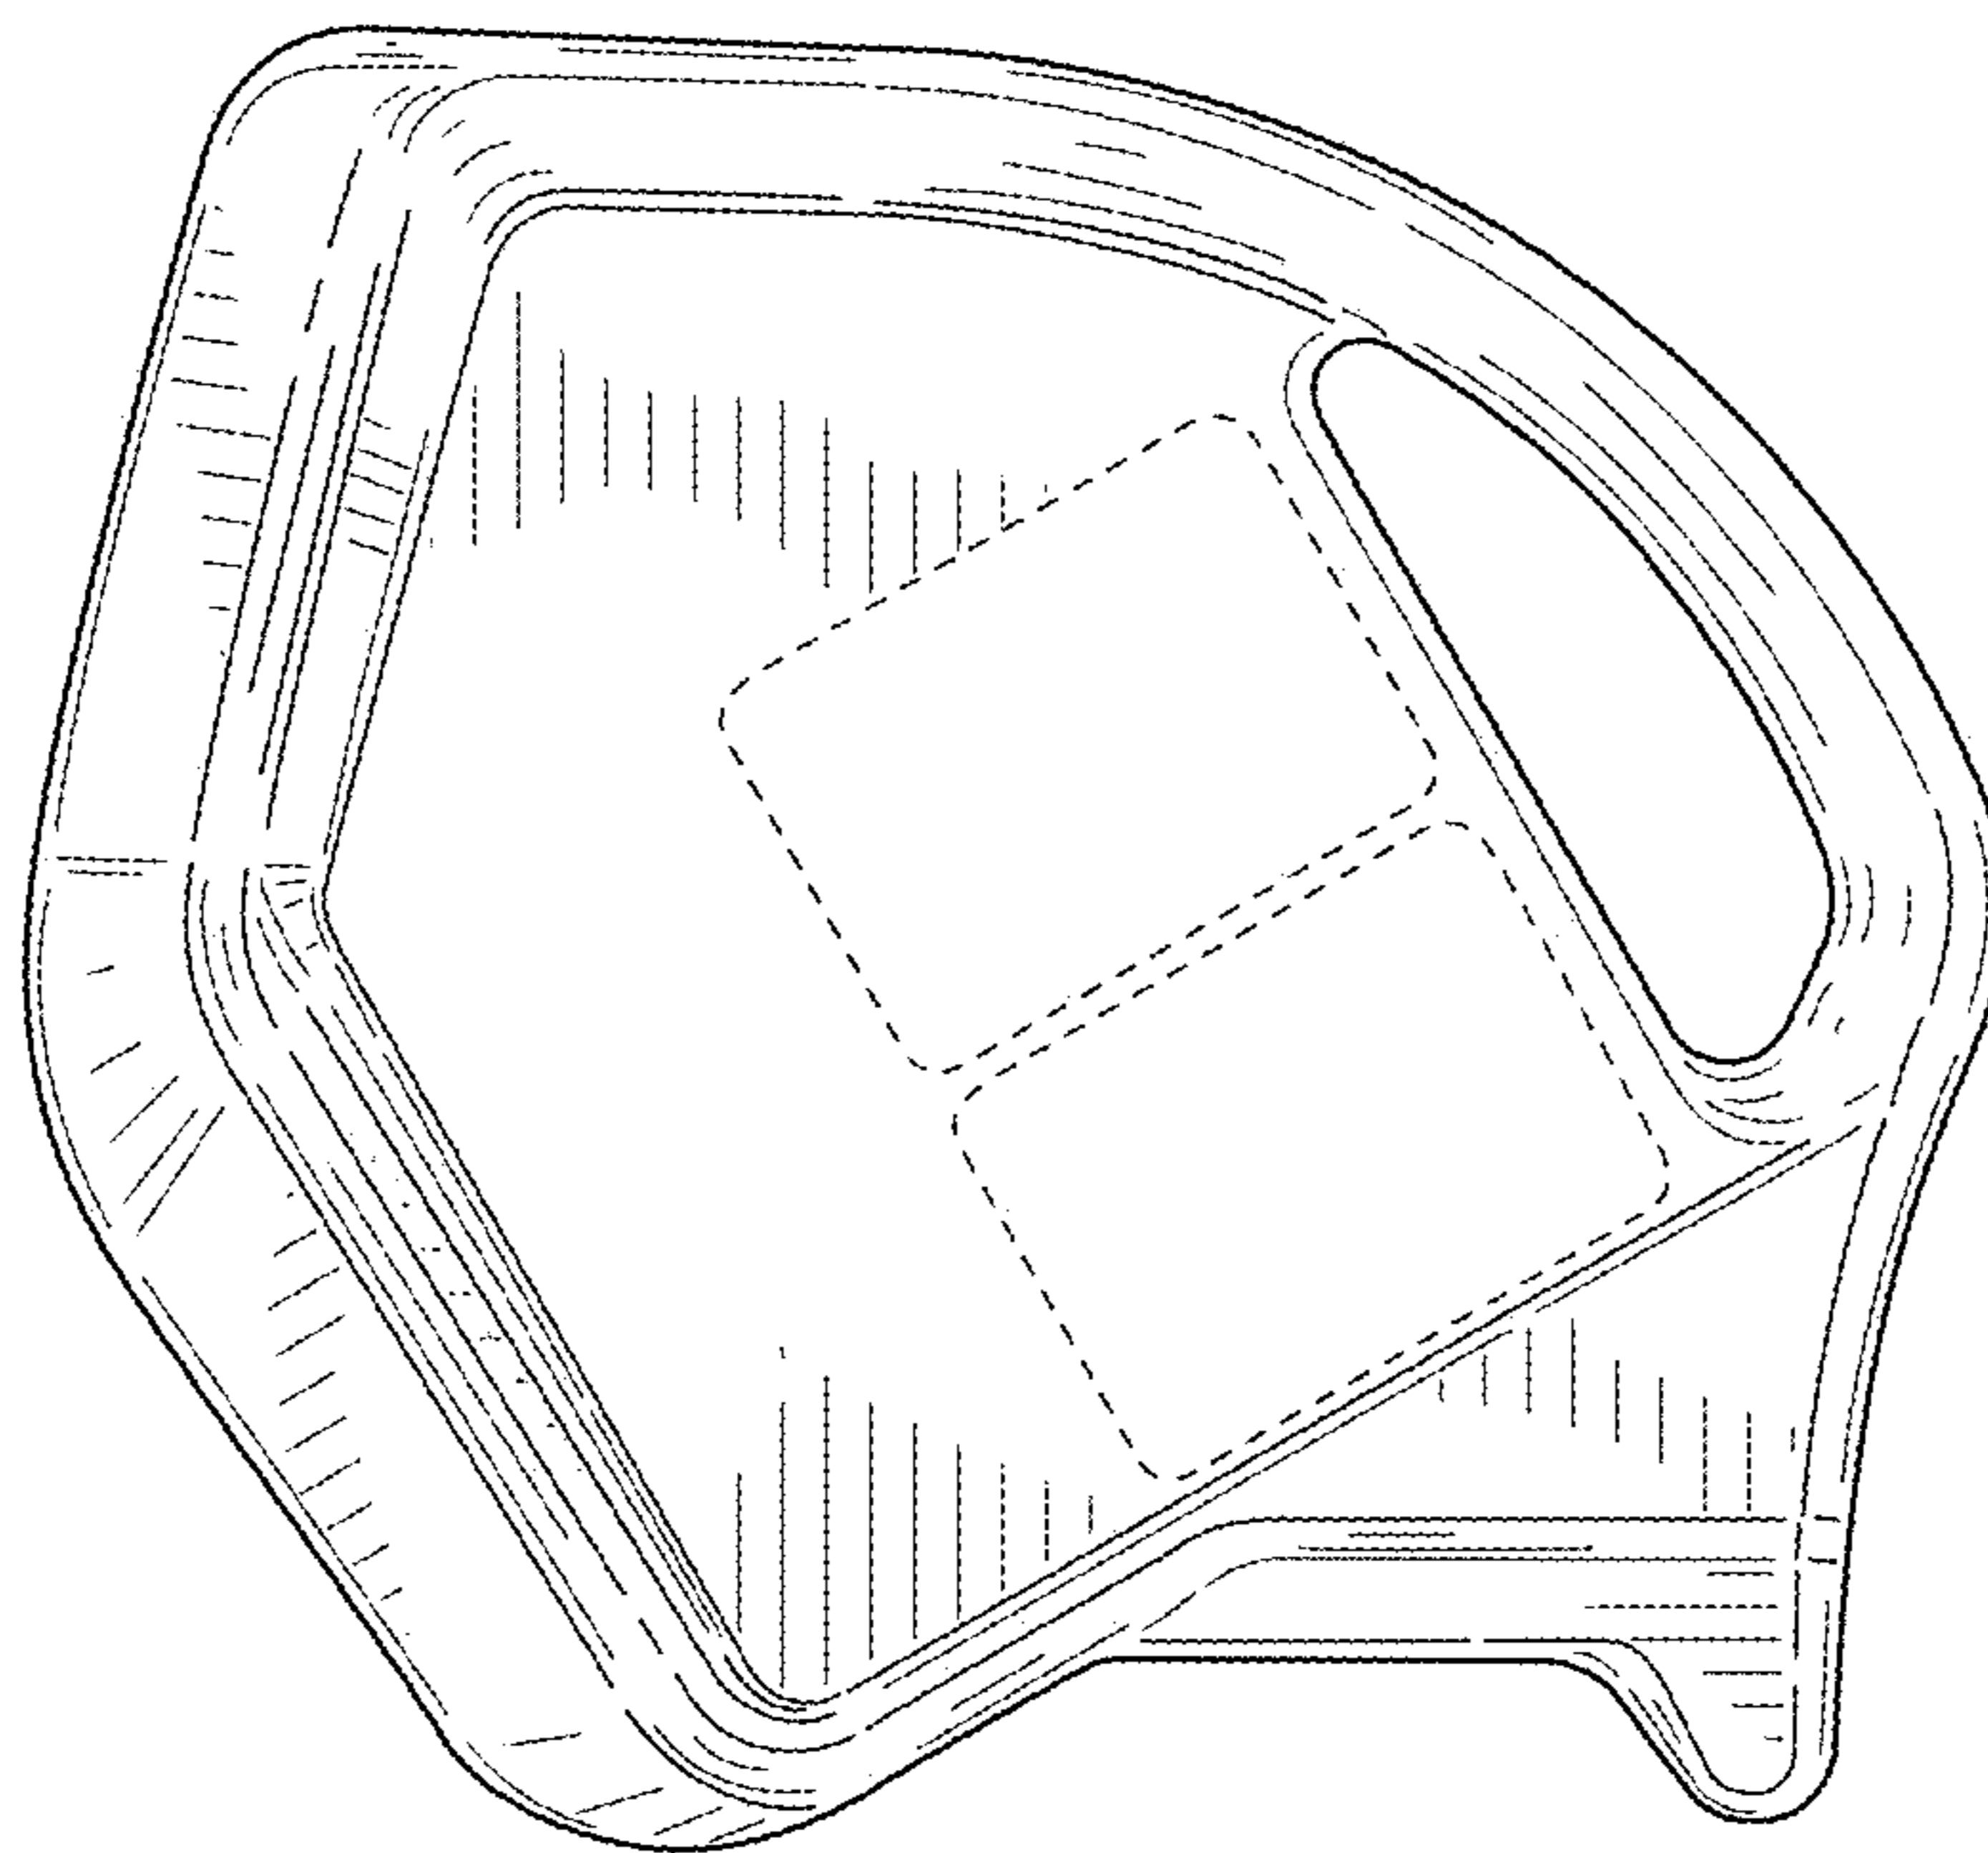


FIG. 10

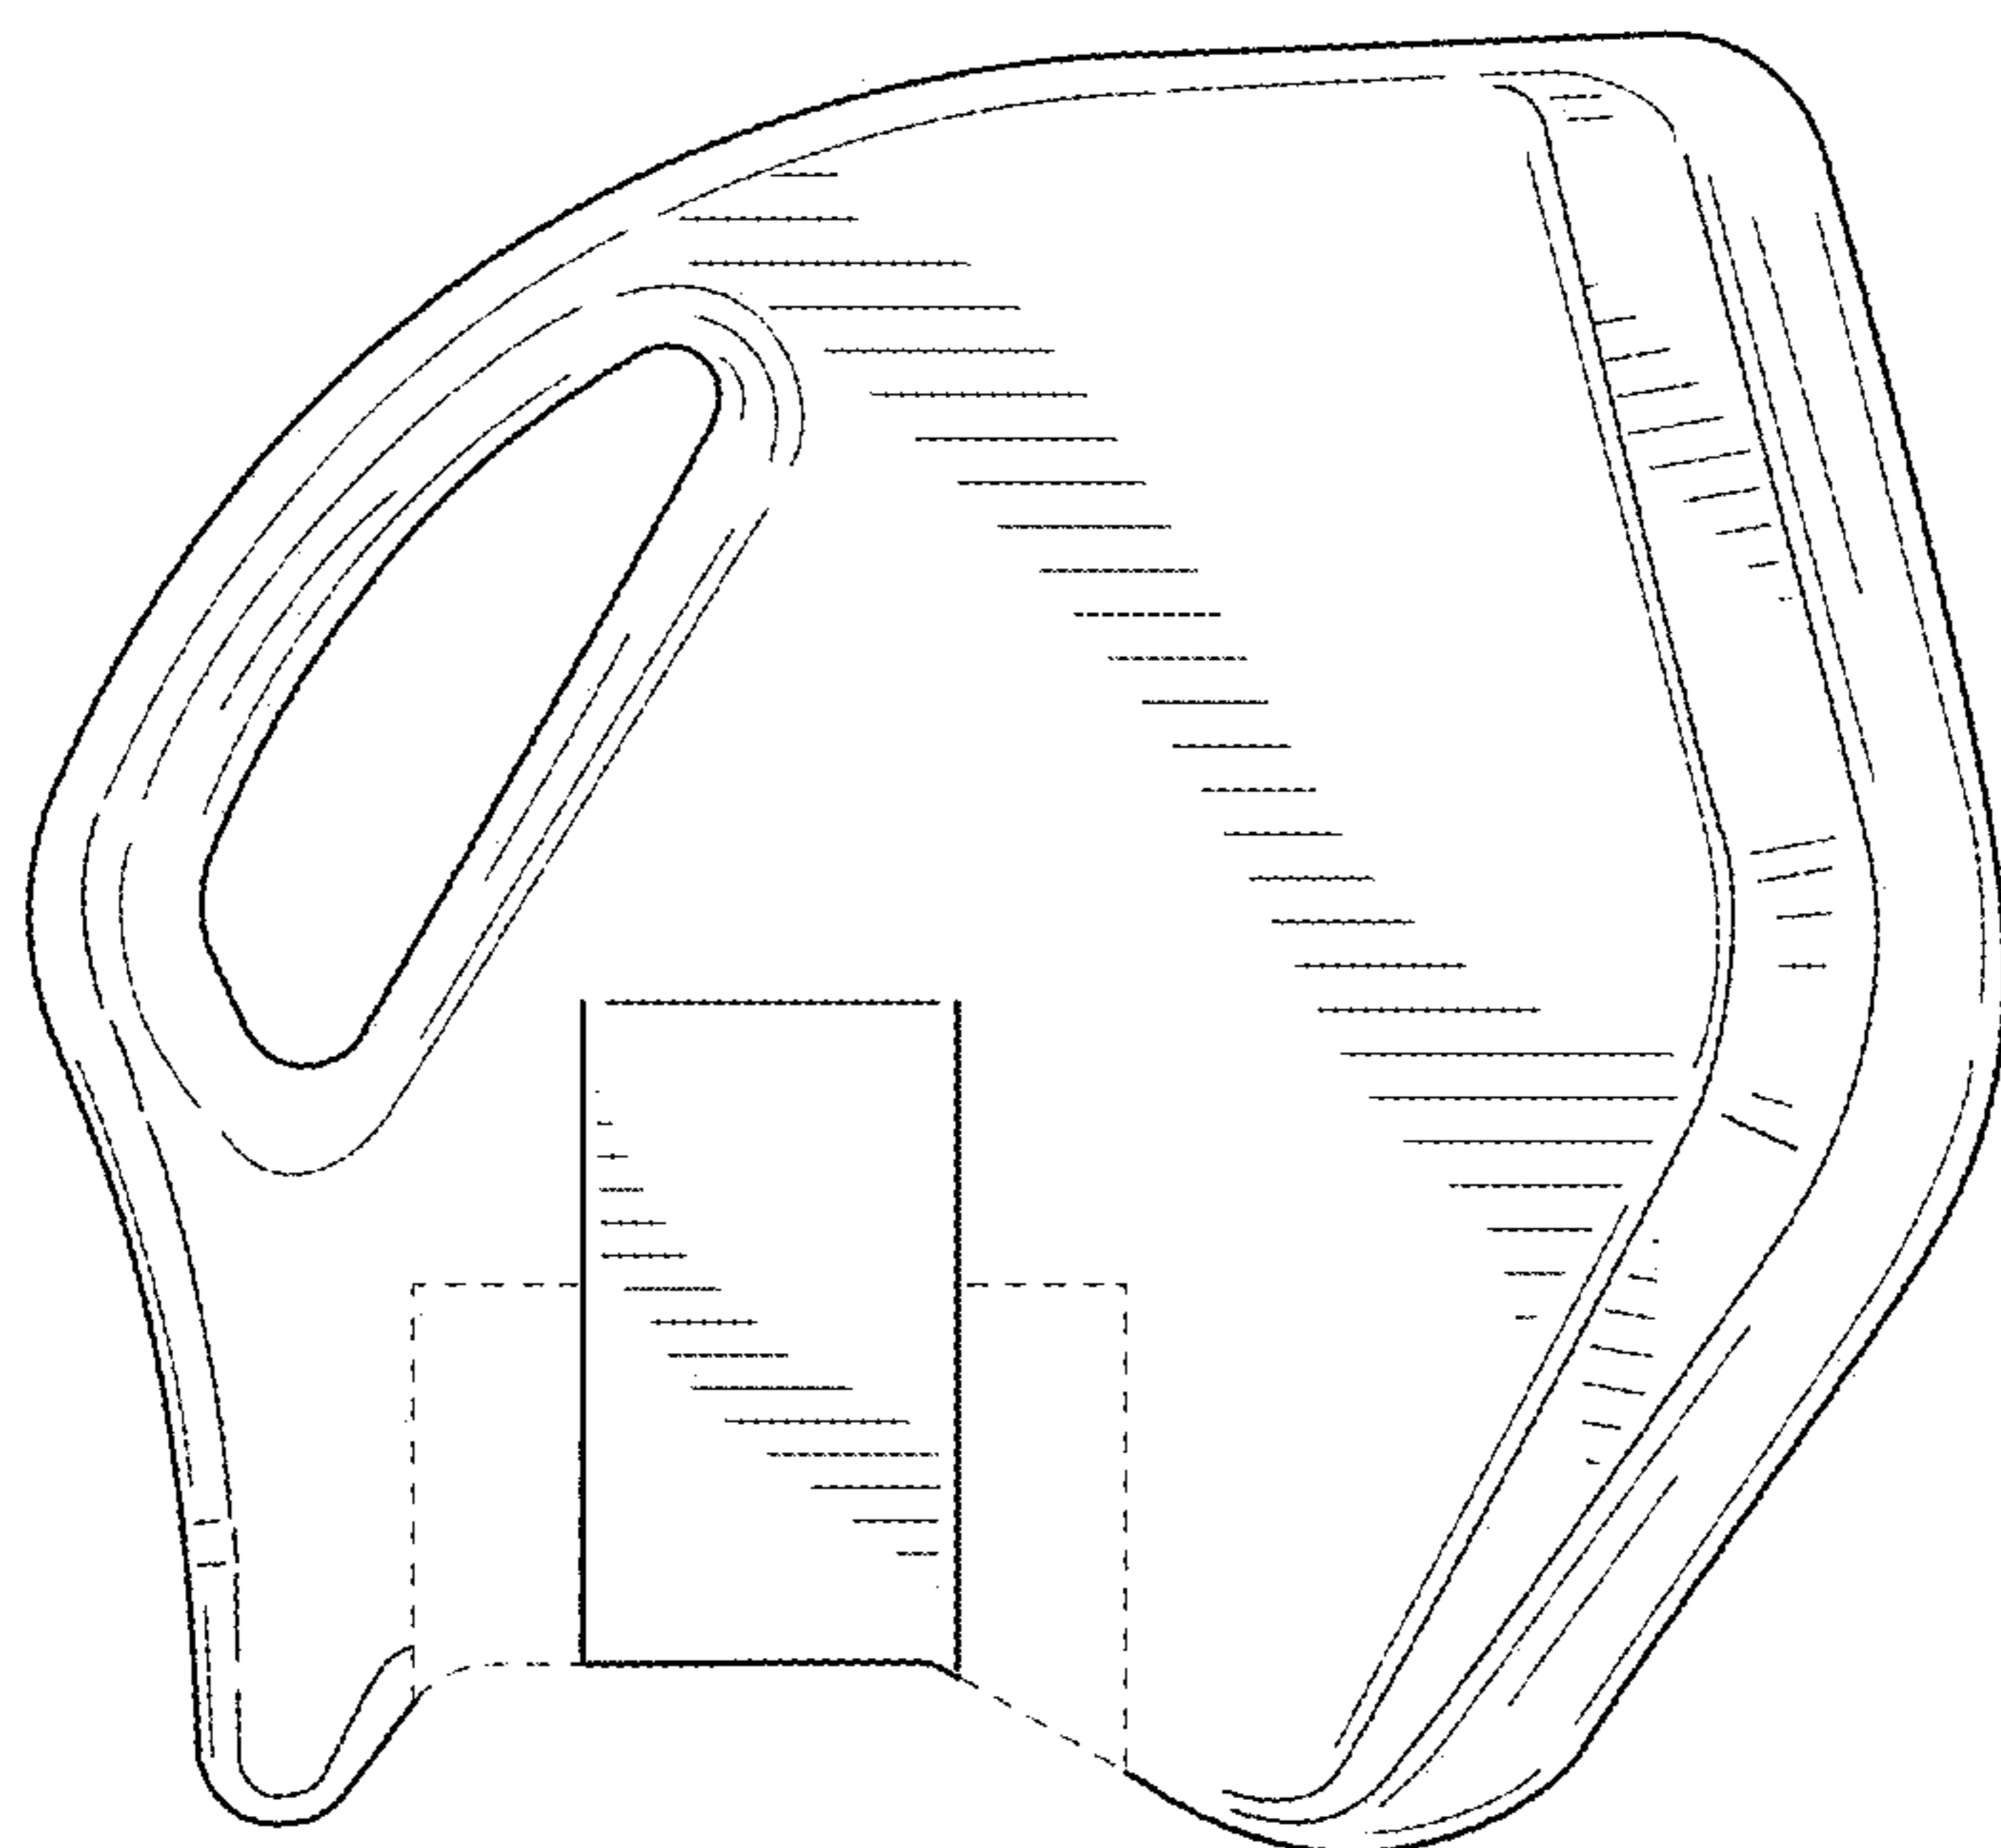


FIG. 11

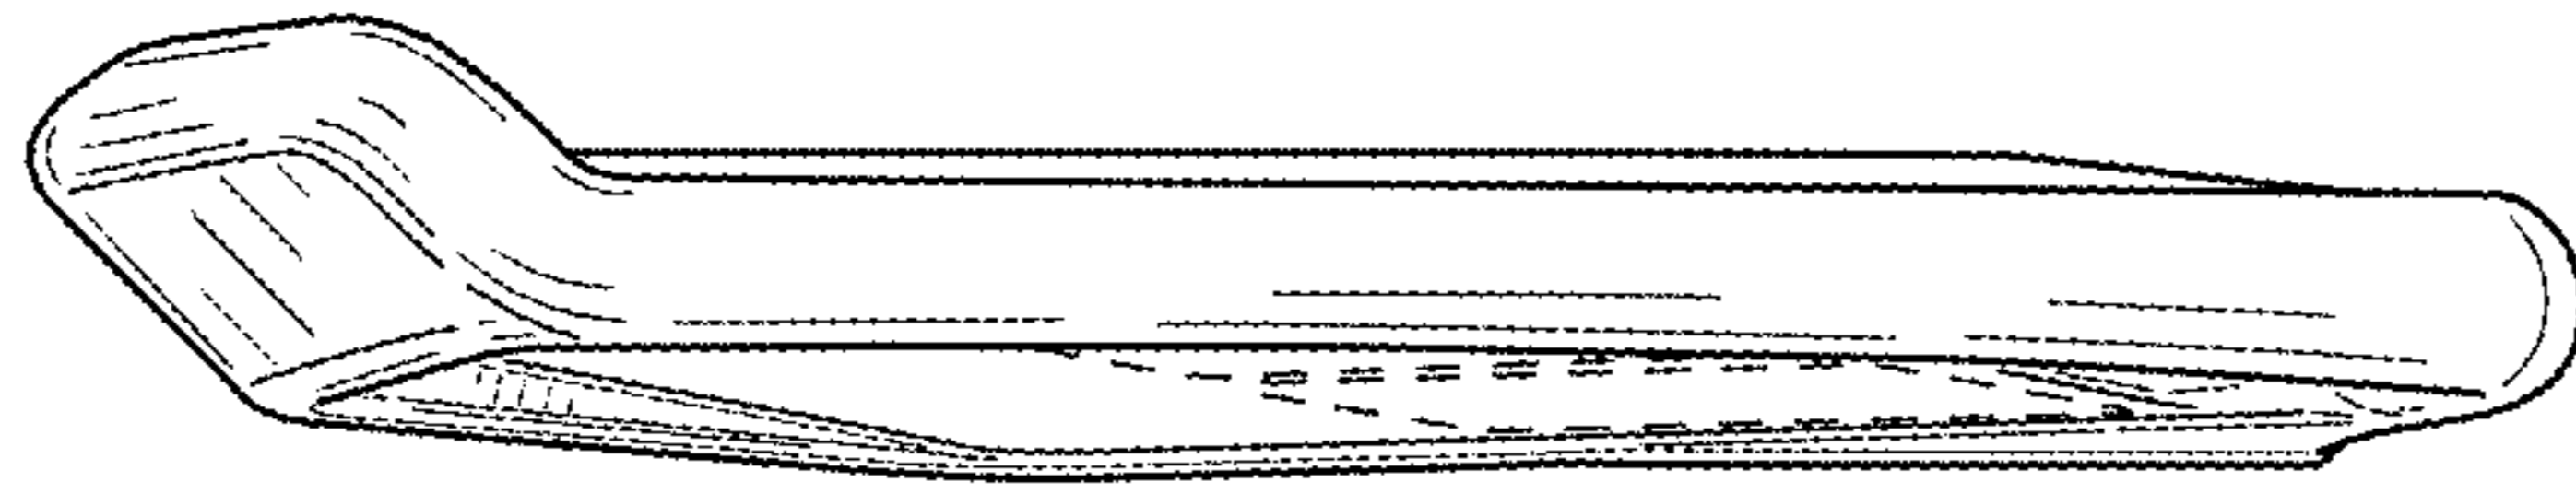


FIG. 12

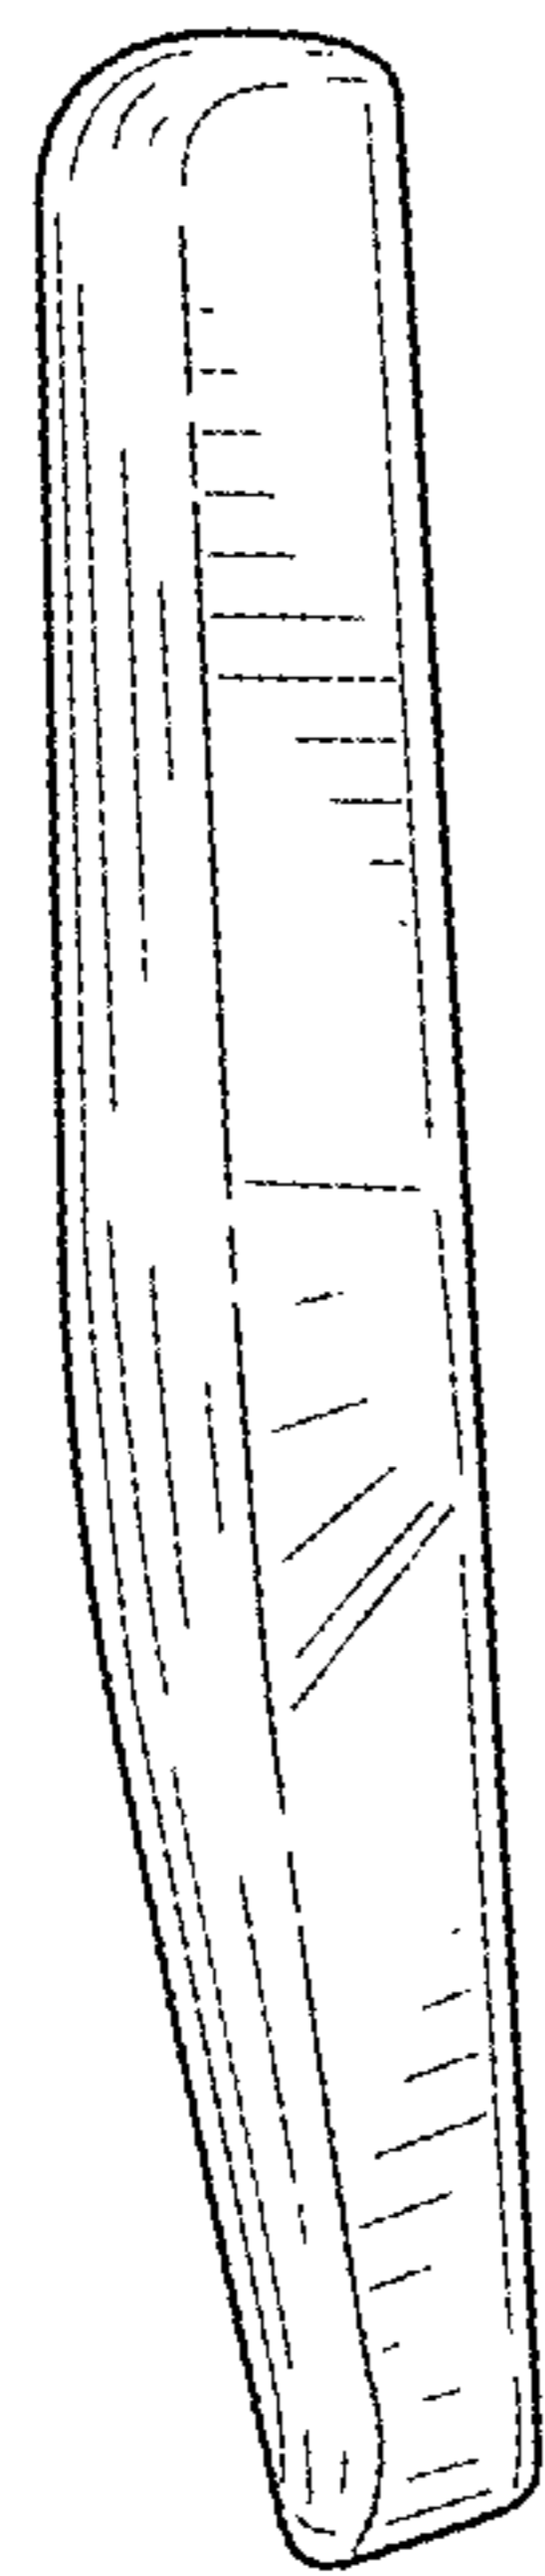


FIG. 13

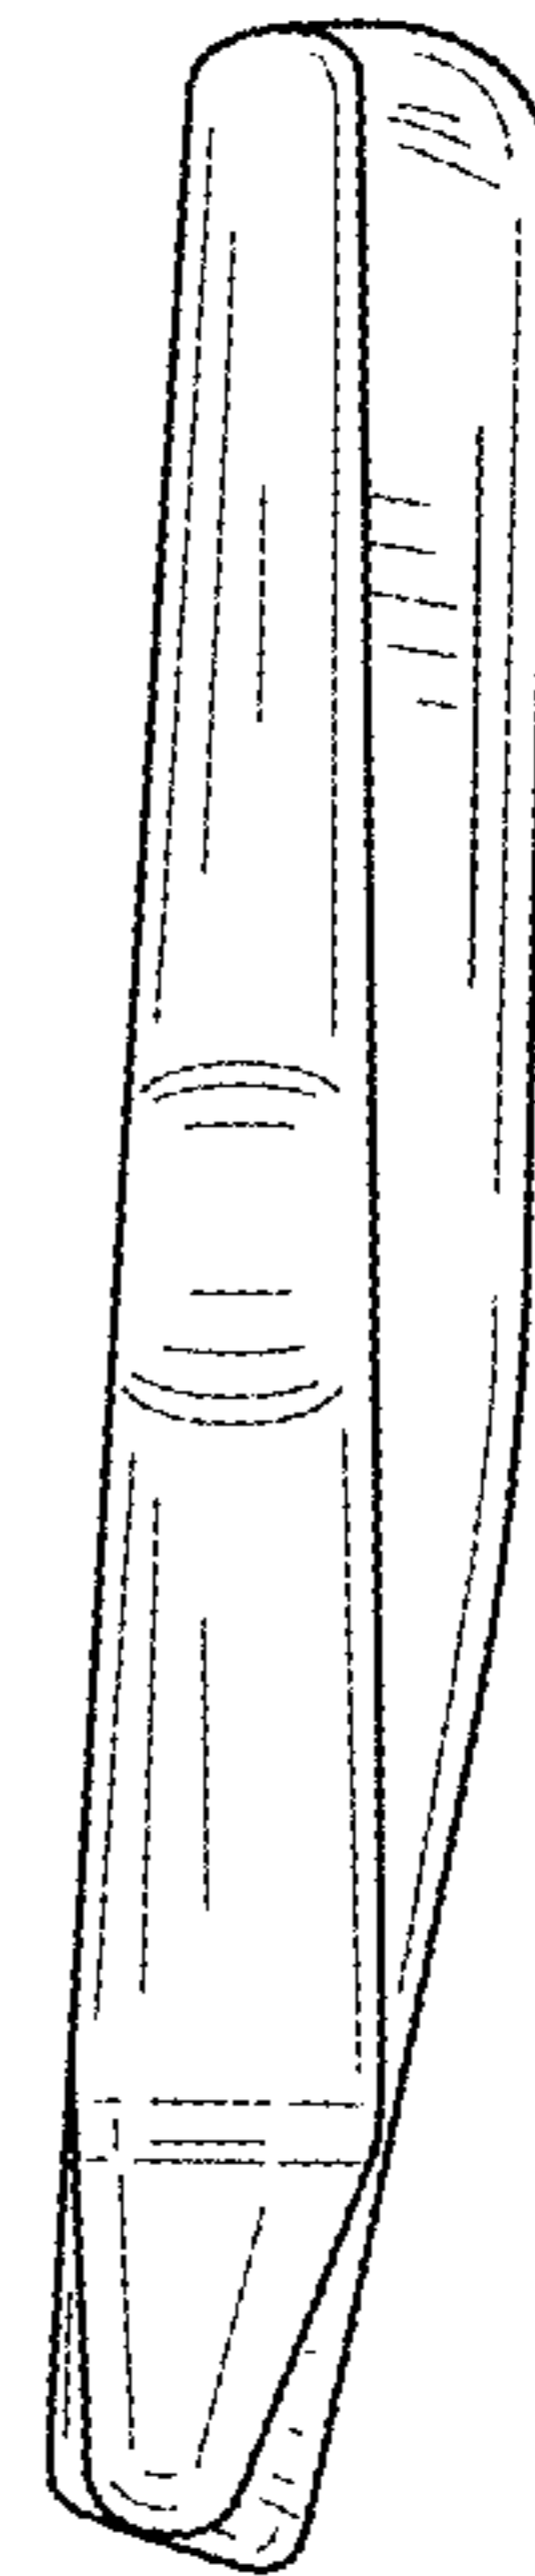


FIG. 14