



US0D1007661S

(12)

United States Design Patent

Maeckelberghe et al.

(10) Patent No.:

US D1,007,661 S

(45) Date of Patent:


** Dec. 12, 2023

- (54) CIRCUIT KIT FOR A HUMIDIFIER
- (71) Applicant: Fisher & Paykel Healthcare Limited, Auckland (NZ)
- (72) Inventors: Thomas Jacques Fernand Maeckelberghe, Auckland (NZ); Gareth James Hobbs, Auckland (NZ); Matthew Liam Buswell, Auckland (NZ); Jason Allan Klenner, Auckland (NZ); David Leon McCauley, Auckland (NZ); Elmo Benson Stoks, Auckland (NZ); Samuel Graham Boggs, Auckland (NZ); Jonathan Andrew George Lambert, Auckland (NZ); James William Stanton, Auckland (NZ)
- (73) Assignee: Fisher & Paykel Healthcare Limited, Auckland (NZ)
- (**) Term: 15 Years
- (21) Appl. No.: 29/788,455
- (22) Filed: May 28, 2021

Related U.S. Application Data

- (62) Division of application No. 29/650,779, filed on Jun. 8, 2018, now Pat. No. Des. 923,768, which is a division of application No. 29/626,135, filed on Nov. 15, 2017, now Pat. No. Des. 822,818, which is a division of application No. 29/625,933, filed on Nov. 14, 2017, now Pat. No. Des. 822,817, which is a division of application No. 29/540,276, filed on Sep. 22, 2015, now Pat. No. Des. 807,995.
- (51) LOC (14) Cl. 23-04
- (52) U.S. Cl. USPC D23/358
- (58) Field of Classification Search USPC D23/364, 366, 333, 332, 355, 356, 359, D23/209, 358; D32/18; D24/110, 129 CPC B01D 46/02; B01D 46/00 See application file for complete search history.

(56) References Cited	
U.S. PATENT DOCUMENTS	
2,516,864 A	8/1950 Gilmore et al.
4,188,081 A	2/1980 Holden et al.
4,621,632 A	11/1986 Bartels et al.
4,686,354 A	8/1987 Makin
D302,040 S	7/1989 Lambert
5,069,635 A	12/1991 Holden et al.
D360,027 S	7/1995 Psaros
5,514,303 A	5/1996 Chiu et al.
D439,326 S	3/2001 Hecker et al.
7,226,302 B2 *	6/2007 Walter A47L 9/246 15/377
D561,890 S *	2/2008 Lithgow D24/110
D585,131 S *	1/2009 Trevor-Wilson D24/110
D628,288 S	11/2010 Row et al.
D629,891 S	12/2010 Virr et al.
D629,892 S	12/2010 Hill et al.
D638,536 S	5/2011 Row et al.
D638,537 S	5/2011 Virr et al.
D638,933 S	5/2011 Hill et al.
D652,916 S	1/2012 Row et al.
D652,917 S	1/2012 Hill et al.
D655,813 S	3/2012 Row
8,240,306 B2	8/2012 Cortez, Jr. et al.
D671,209 S	11/2012 Row et al.
D675,730 S	2/2013 Lithgow et al.
D677,789 S *	3/2013 Row D24/129
8,453,640 B2	6/2013 Martin et al.
D691,712 S *	10/2013 Judson D24/110.1
D710,493 S	8/2014 Wu
8,905,031 B2	12/2014 Barlow
D737,953 S	9/2015 Wells et al.
D741,477 S	10/2015 Rogers
D742,508 S	11/2015 Row et al.
D751,687 S	3/2016 Daly
D751,688 S	3/2016 Daly
D761,422 S	7/2016 Row et al.
D762,843 S	8/2016 Formica et al.
9,669,124 B2	6/2017 Leyva et al.
D805,630 S *	12/2017 Formica D24/110
D807,995 S	1/2018 Maeckelberghe et al.
D808,516 S	1/2018 Edwards et al.
D809,124 S	1/2018 Bertinetti et al.
D822,817 S	7/2018 Maeckelberghe et al.
D822,818 S *	7/2018 Maeckelberghe D24/110
10,080,856 B2	9/2018 McLaren et al.
D841,147 S	2/2019 McCool et al.
D841,148 S	2/2019 Stoks et al.
D847,326 S	4/2019 Eury et al.
D849,232 S *	5/2019 Formica D24/110

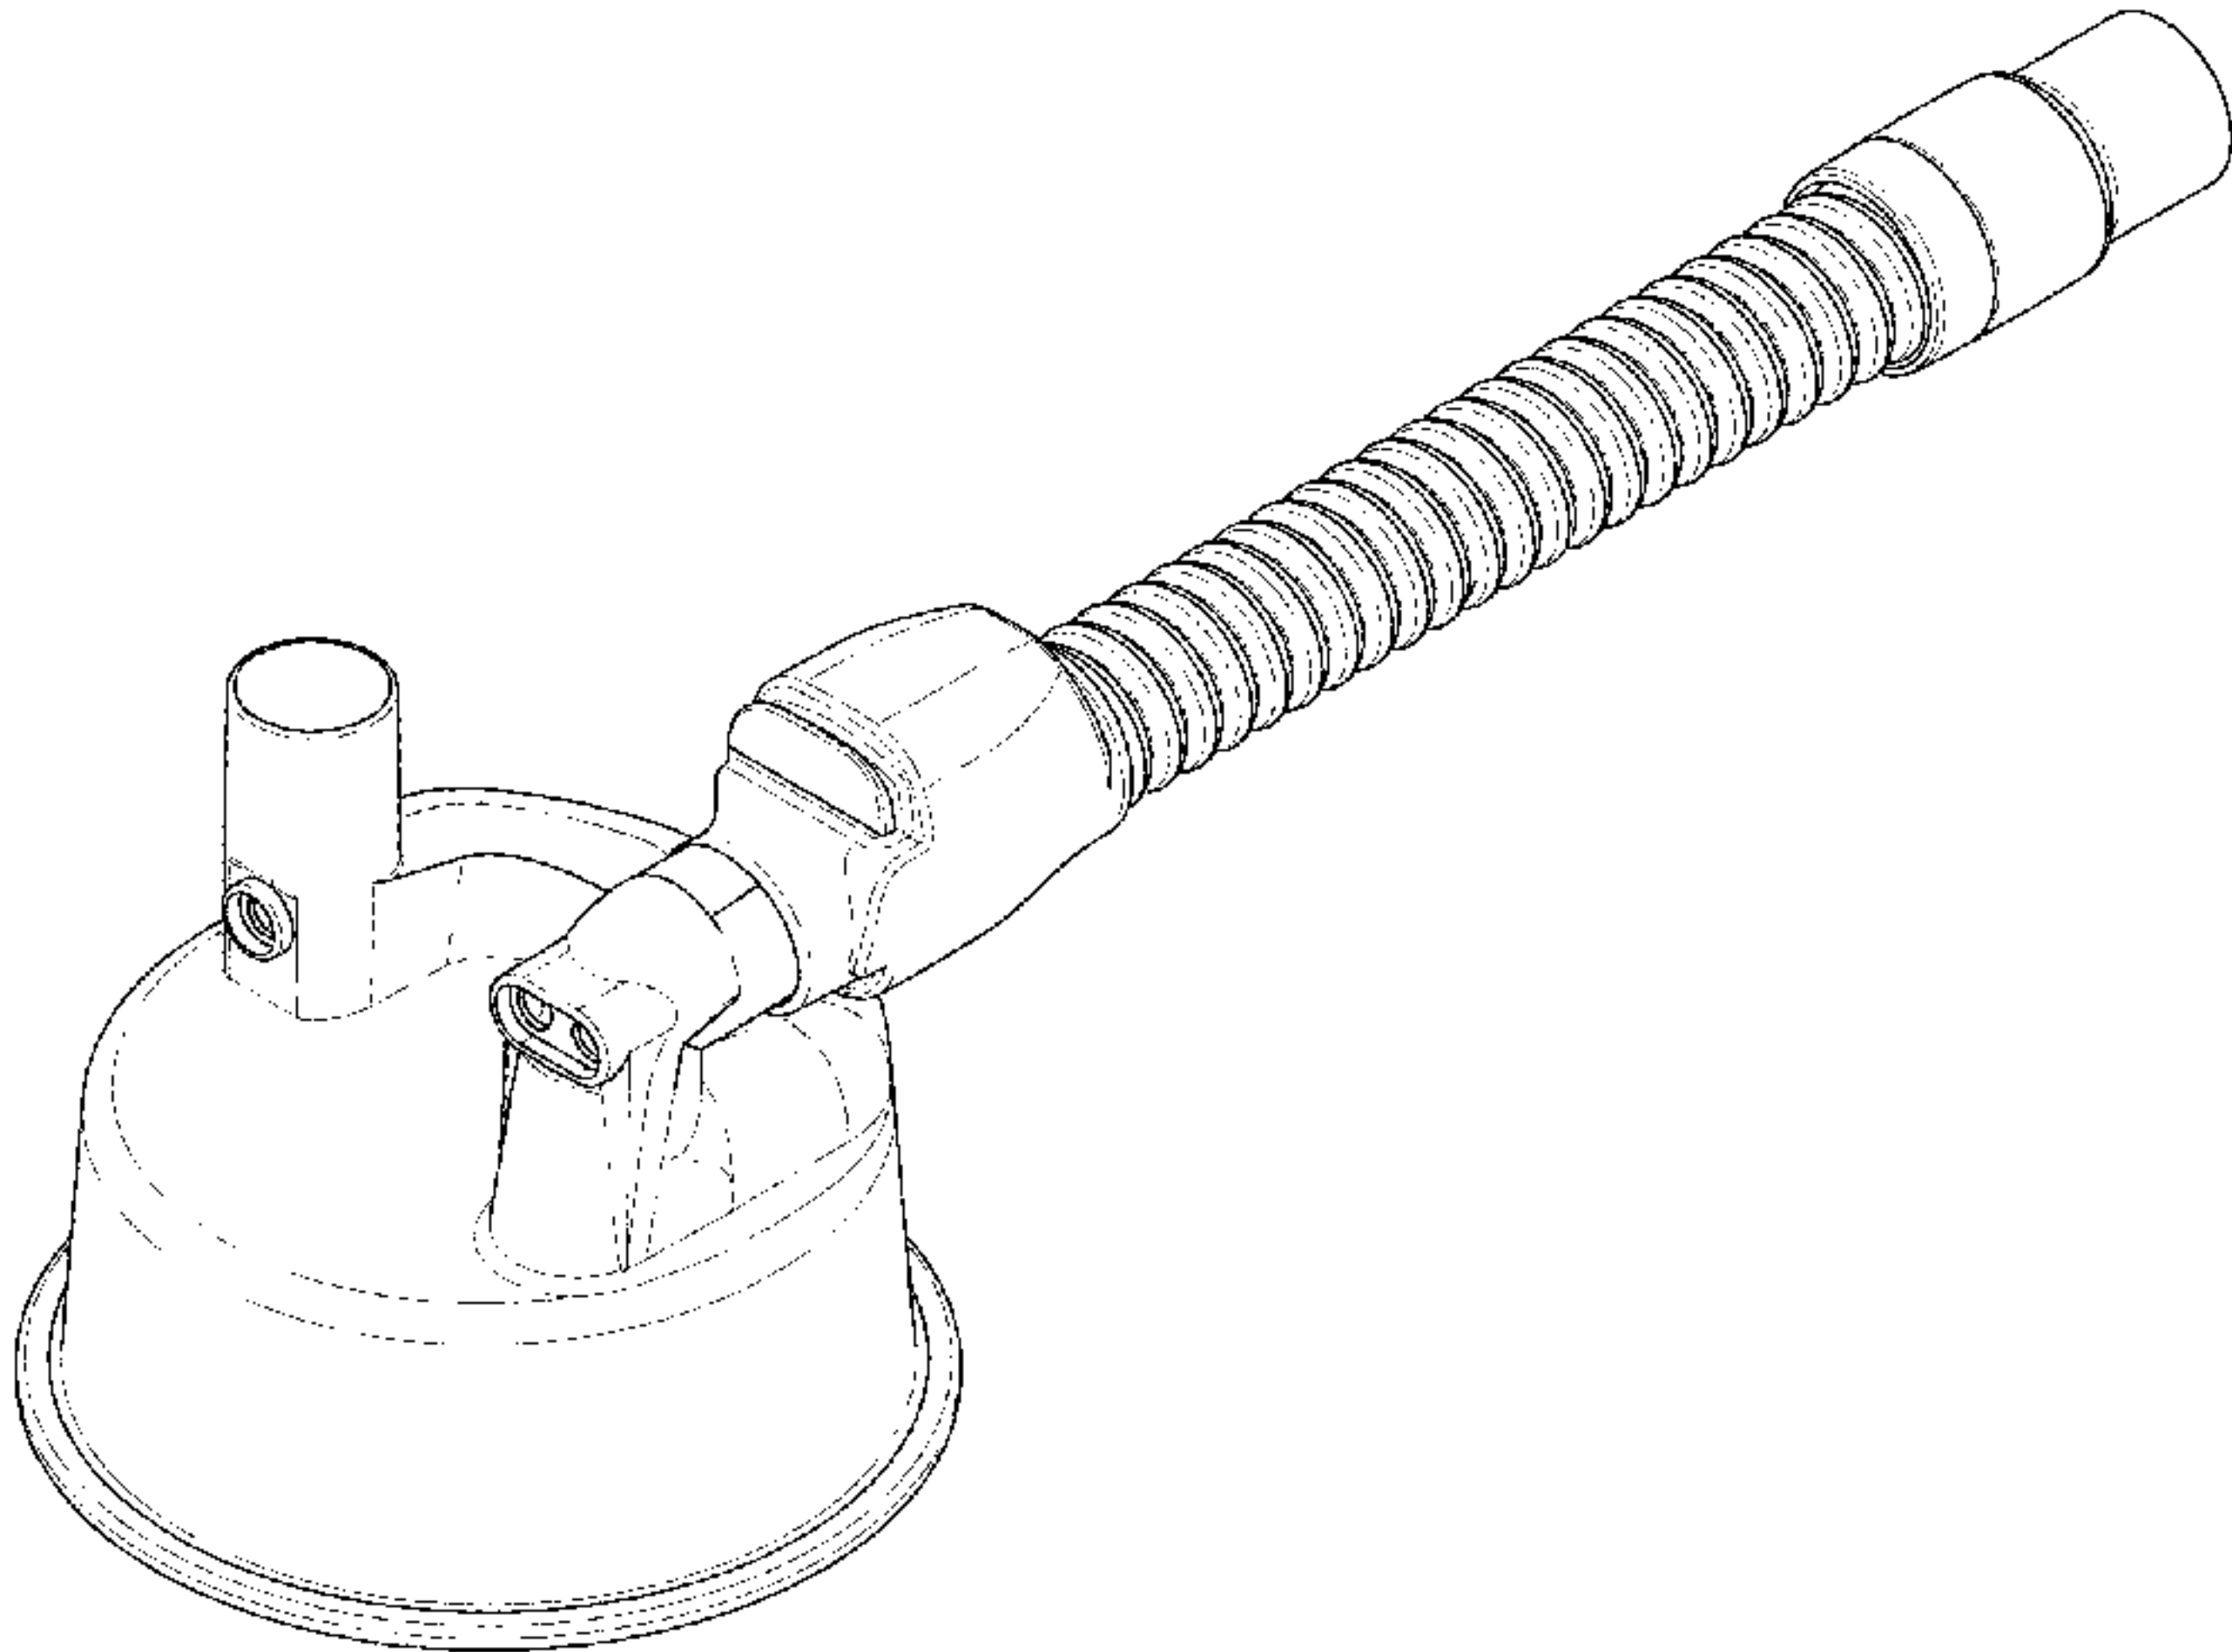

D861,854 S *	10/2019	Ormrod	D24/110
10,449,318 B2	10/2019	Graham et al.	
10,456,546 B2	10/2019	McLaren et al.	
10,456,547 B2	10/2019	Miller et al.	
D874,645 S	2/2020	McCool et al.	
D878,546 S *	3/2020	Formica	D24/110
D880,686 S	4/2020	Stoks et al.	
10,688,270 B2	6/2020	Sims et al.	
D901,673 S *	11/2020	Gordon	D24/110.4
D905,215 S *	12/2020	Herweck	D23/332
10,850,059 B2	12/2020	Bencke et al.	
D923,169 S *	6/2021	McCool	D24/110
D923,768 S *	6/2021	Maeckelberghe	D23/358
D958,968 S *	7/2022	Hobbs	D24/110.2
11,446,462 B2 *	9/2022	Holyoake	A61M 16/024
D968,587 S *	11/2022	Holyoake	D24/110
D973,862 S *	12/2022	How	D24/110
D974,551 S *	1/2023	Mosen	D24/129
2003/0236015 A1 *	12/2003	Edirisuriya	A61M 16/16 439/191
2009/0025724 A1	1/2009	Herron, Jr.	
2009/0136341 A1	5/2009	Kenyon	
2009/0266361 A1	10/2009	Bilger et al.	
2011/0308520 A1 *	12/2011	McAuley	A61M 16/0683 128/207.18
2012/0227738 A1	9/2012	Virr et al.	
2012/0304994 A1	12/2012	Kwok	
2013/0008440 A1	1/2013	Maurer et al.	
2013/0047987 A1	2/2013	Mays	
2013/0333701 A1	12/2013	Herron	
2014/0053939 A1 *	2/2014	Kaye	F16L 33/34 138/109
2014/0158133 A1	6/2014	Acosta	
2015/0108670 A1 *	4/2015	Magee	A61M 16/1085 261/142
2015/0128944 A1	5/2015	Buechi	
2015/0277733 A1	10/2015	Schwaibold	
2015/0283350 A1	10/2015	Miller et al.	
2015/0306326 A1	10/2015	Graham	
2015/0306332 A1	10/2015	Bafle	
2017/0000967 A1	1/2017	Sims et al.	
2017/0100556 A1	4/2017	Munkelt et al.	
2017/0209610 A1	7/2017	Leyva et al.	
2017/0304578 A1	10/2017	Stoks	
2017/0361051 A1	12/2017	Eifler	
2017/0368285 A1 *	12/2017	Wood	A61M 16/0683
2018/0214659 A1	8/2018	Forrester	
2019/0022344 A1	1/2019	Lau et al.	
2019/0076620 A1	3/2019	Stoks	
2019/0336627 A1	11/2019	Lucio	
2019/0344037 A1	11/2019	Forrester	
2019/0388640 A1	12/2019	Graham et al.	
2020/0016359 A1	1/2020	Miller et al.	
2020/0093948 A1	3/2020	Miko et al.	
2020/0114113 A1	4/2020	Hermez	
2020/0129722 A1	4/2020	Foote et al.	
2020/0147334 A1	5/2020	Gray	
2020/0147336 A1	5/2020	Hobbs et al.	
2020/0171186 A1	6/2020	Leyva et al.	
2020/0330718 A1	10/2020	Forrester et al.	
2021/0038852 A1	2/2021	Bencke et al.	

FOREIGN PATENT DOCUMENTS

CN	102762247 B	8/2015
WO	WO 2012/164407 A1	12/2012
WO	WO 2014/077706 A1	5/2014
WO	WO 2014/088430 A1	6/2014
WO	WO 2015/142192 A1	9/2015
WO	WO2017/043981 A1	3/2017

OTHER PUBLICATIONS

Filters Reduce the Risk of Bacterial Transmission from Contaminated Heated Humidifiers Used with CPAP for Obstructive Sleep Apnea, posted to [ncbi.nlm.nih.gov](https://www.ncbi.nlm.nih.gov/pmc/articles/PMC2556912/). Available date: Dec. 15, 2007 [site visited Jan. 9, 2023] Available: <<https://www.ncbi.nlm.nih.gov/pmc/articles/PMC2556912/>> (Year: 2007).*

U.S. Appl. No. 29/728,612, filed Mar. 19, 2020, Stoks et al..

U.S. Appl. No. 29/788,418, filed May 21, 2021, McCool et al..

Climate Line Air Heated Tube for Resmed Airsense by ResMed, posted to [amazon.com](https://www.amazon.com/ResMed-Climate-AirSense-10-AirCurve/dp/B00NN7KMG4/ref=sr_1_6?dchild=1&keywords=CPAP+tube&qid=1614028657&s=hpc&sr+1-6). Available date: Sep. 11, 2014 [site visited Feb. 22, 2021] Available: <https://www.amazon.com/ResMed-Climate-AirSense-10-AirCurve/dp/B00NN7KMG4/ref=sr_1_6?dchild=1&keywords=CPAP+tube&qid=1614028657&s=hpc&sr+1-6> (Year: 2014).

International Standard, ISO 11664-4, dated Nov. 1, 2008; 18 pages.

News Release; Airvo Nasal High Flow System; May 12, 2015; 2 pages.

* cited by examiner

Primary Examiner — Kevin K Rudzinski
(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) CLAIM

The ornamental design for a circuit kit for a humidifier, as shown and described.

DESCRIPTION

FIG. 1 is a top, rear and side perspective view of a circuit kit for a humidifier showing a tubing assembly connected to a chamber embodying our new design;

FIG. 2 is a rear view thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a first side view thereof;

FIG. 5 is a second side view thereof;

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

Broken lines are used to illustrate features of the circuit kit for a humidifier which form no part of the claimed design.

1 Claim, 7 Drawing Sheets

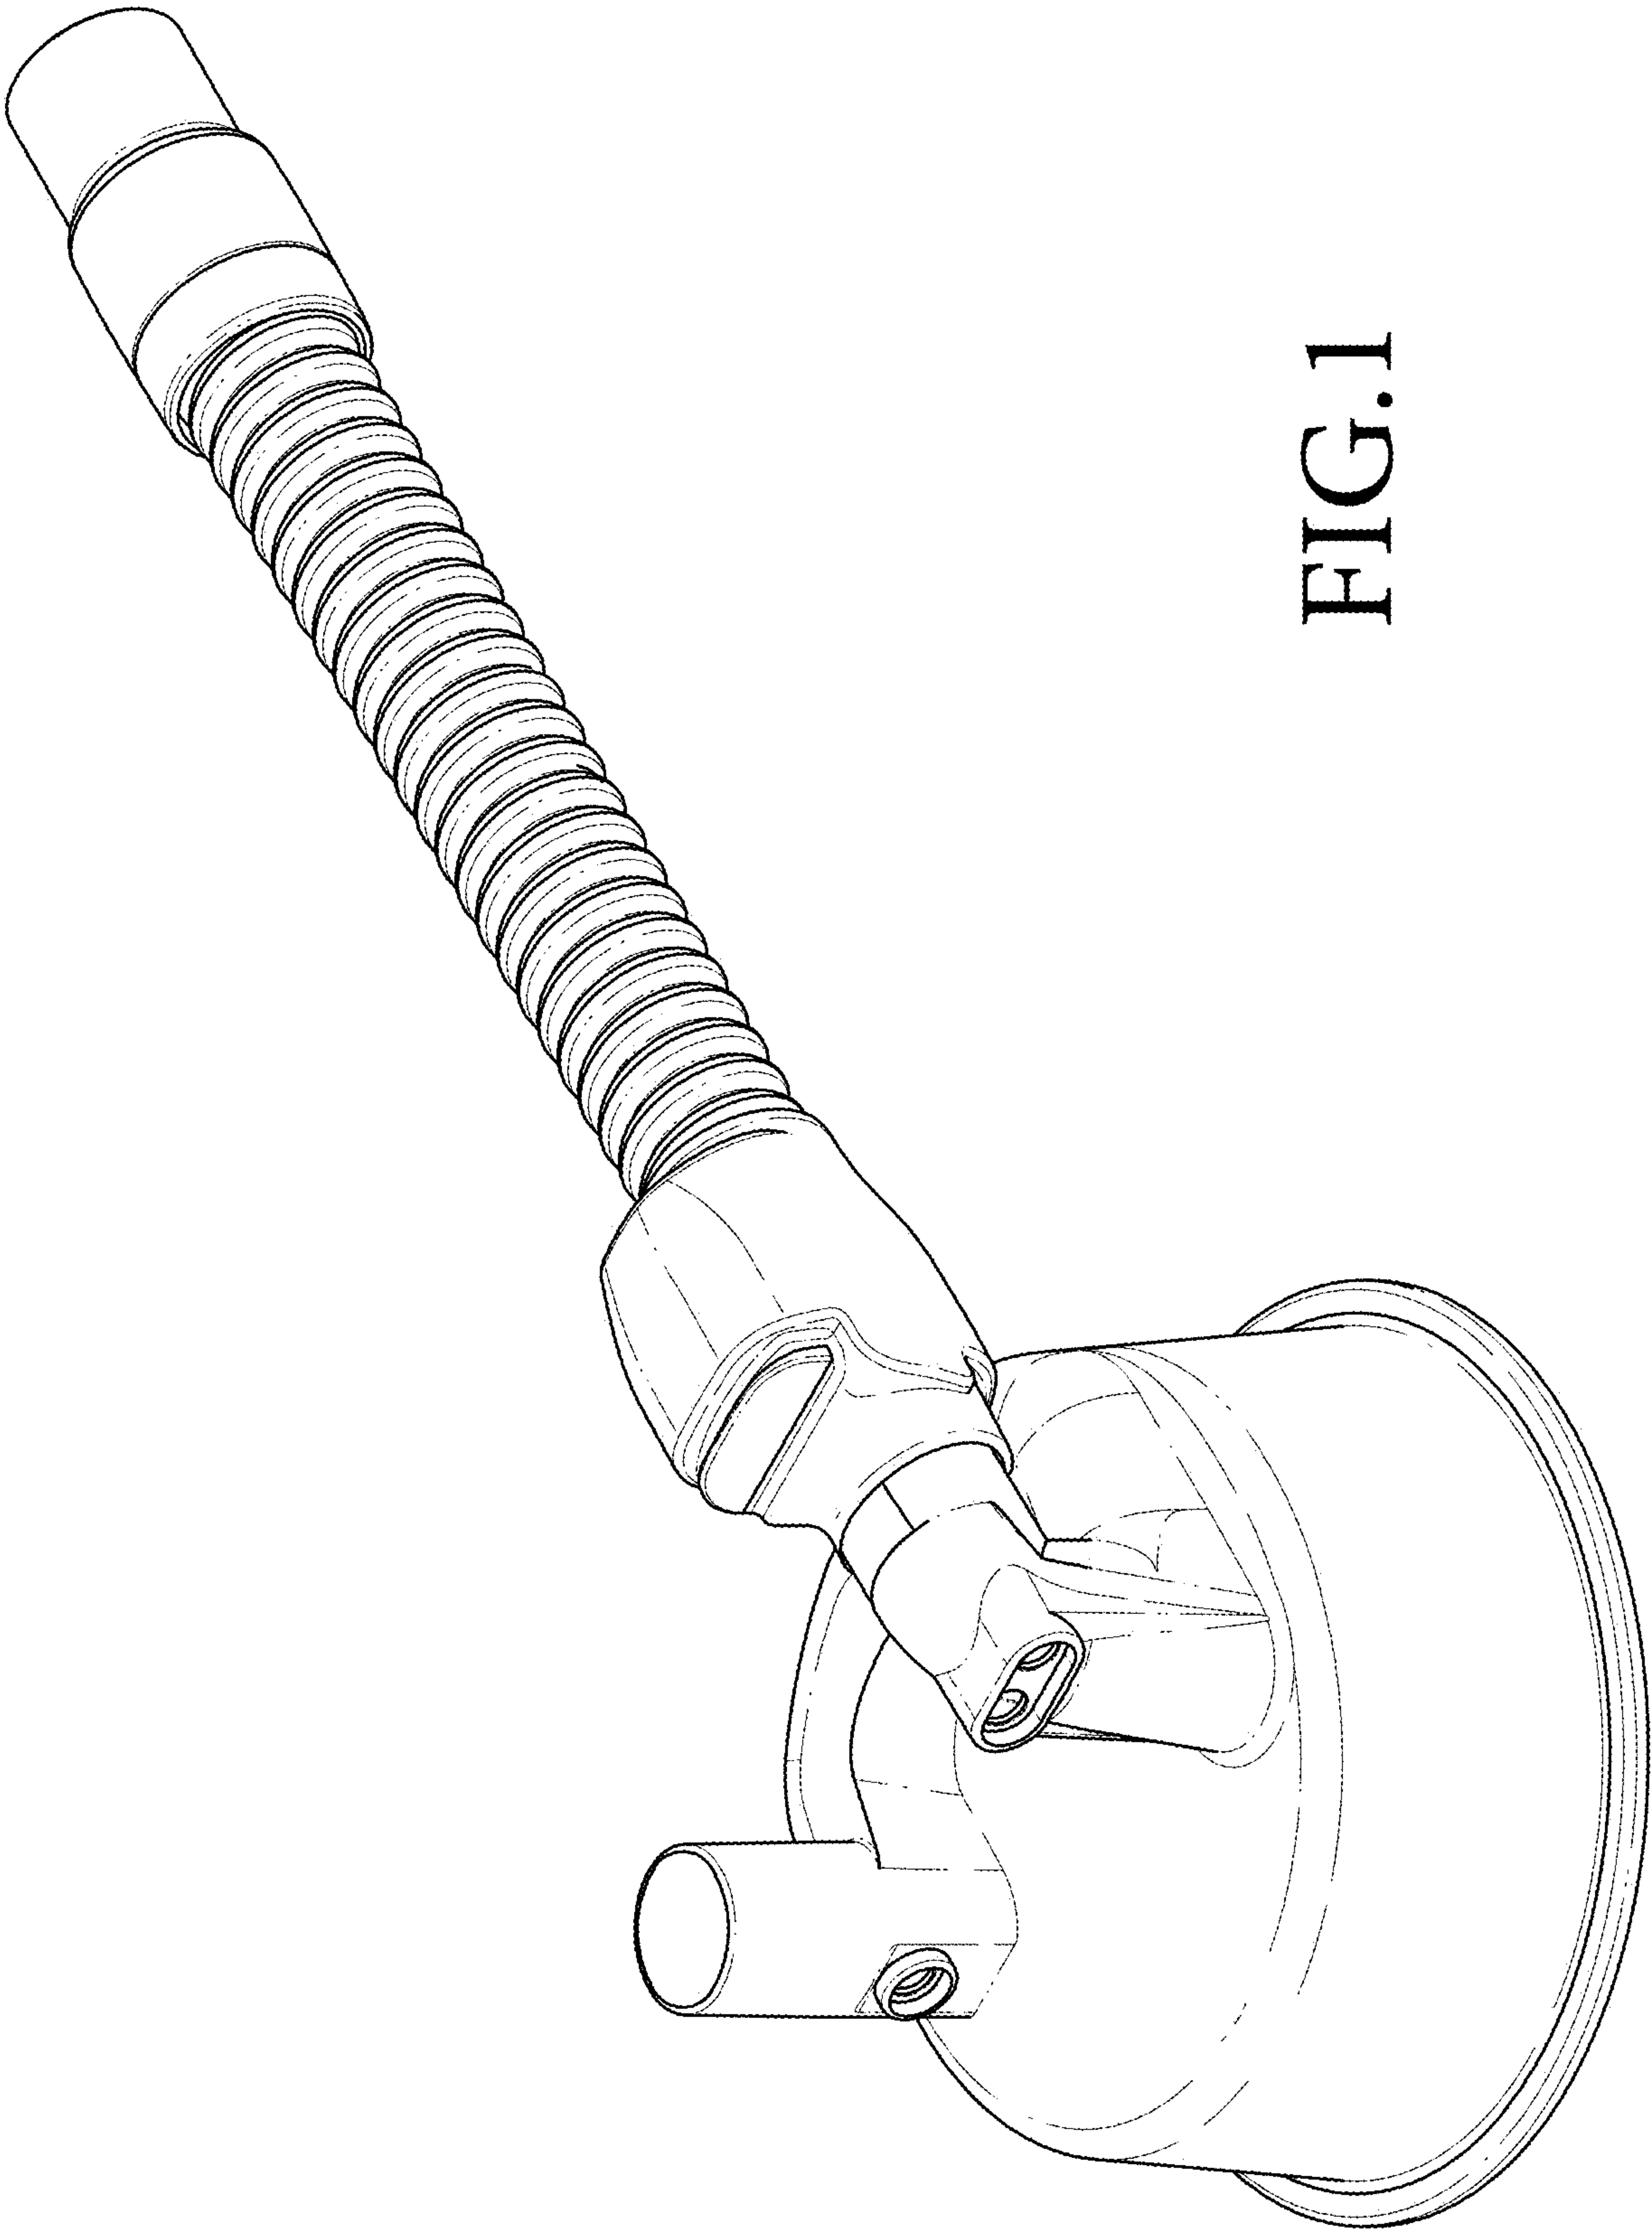


FIG.1

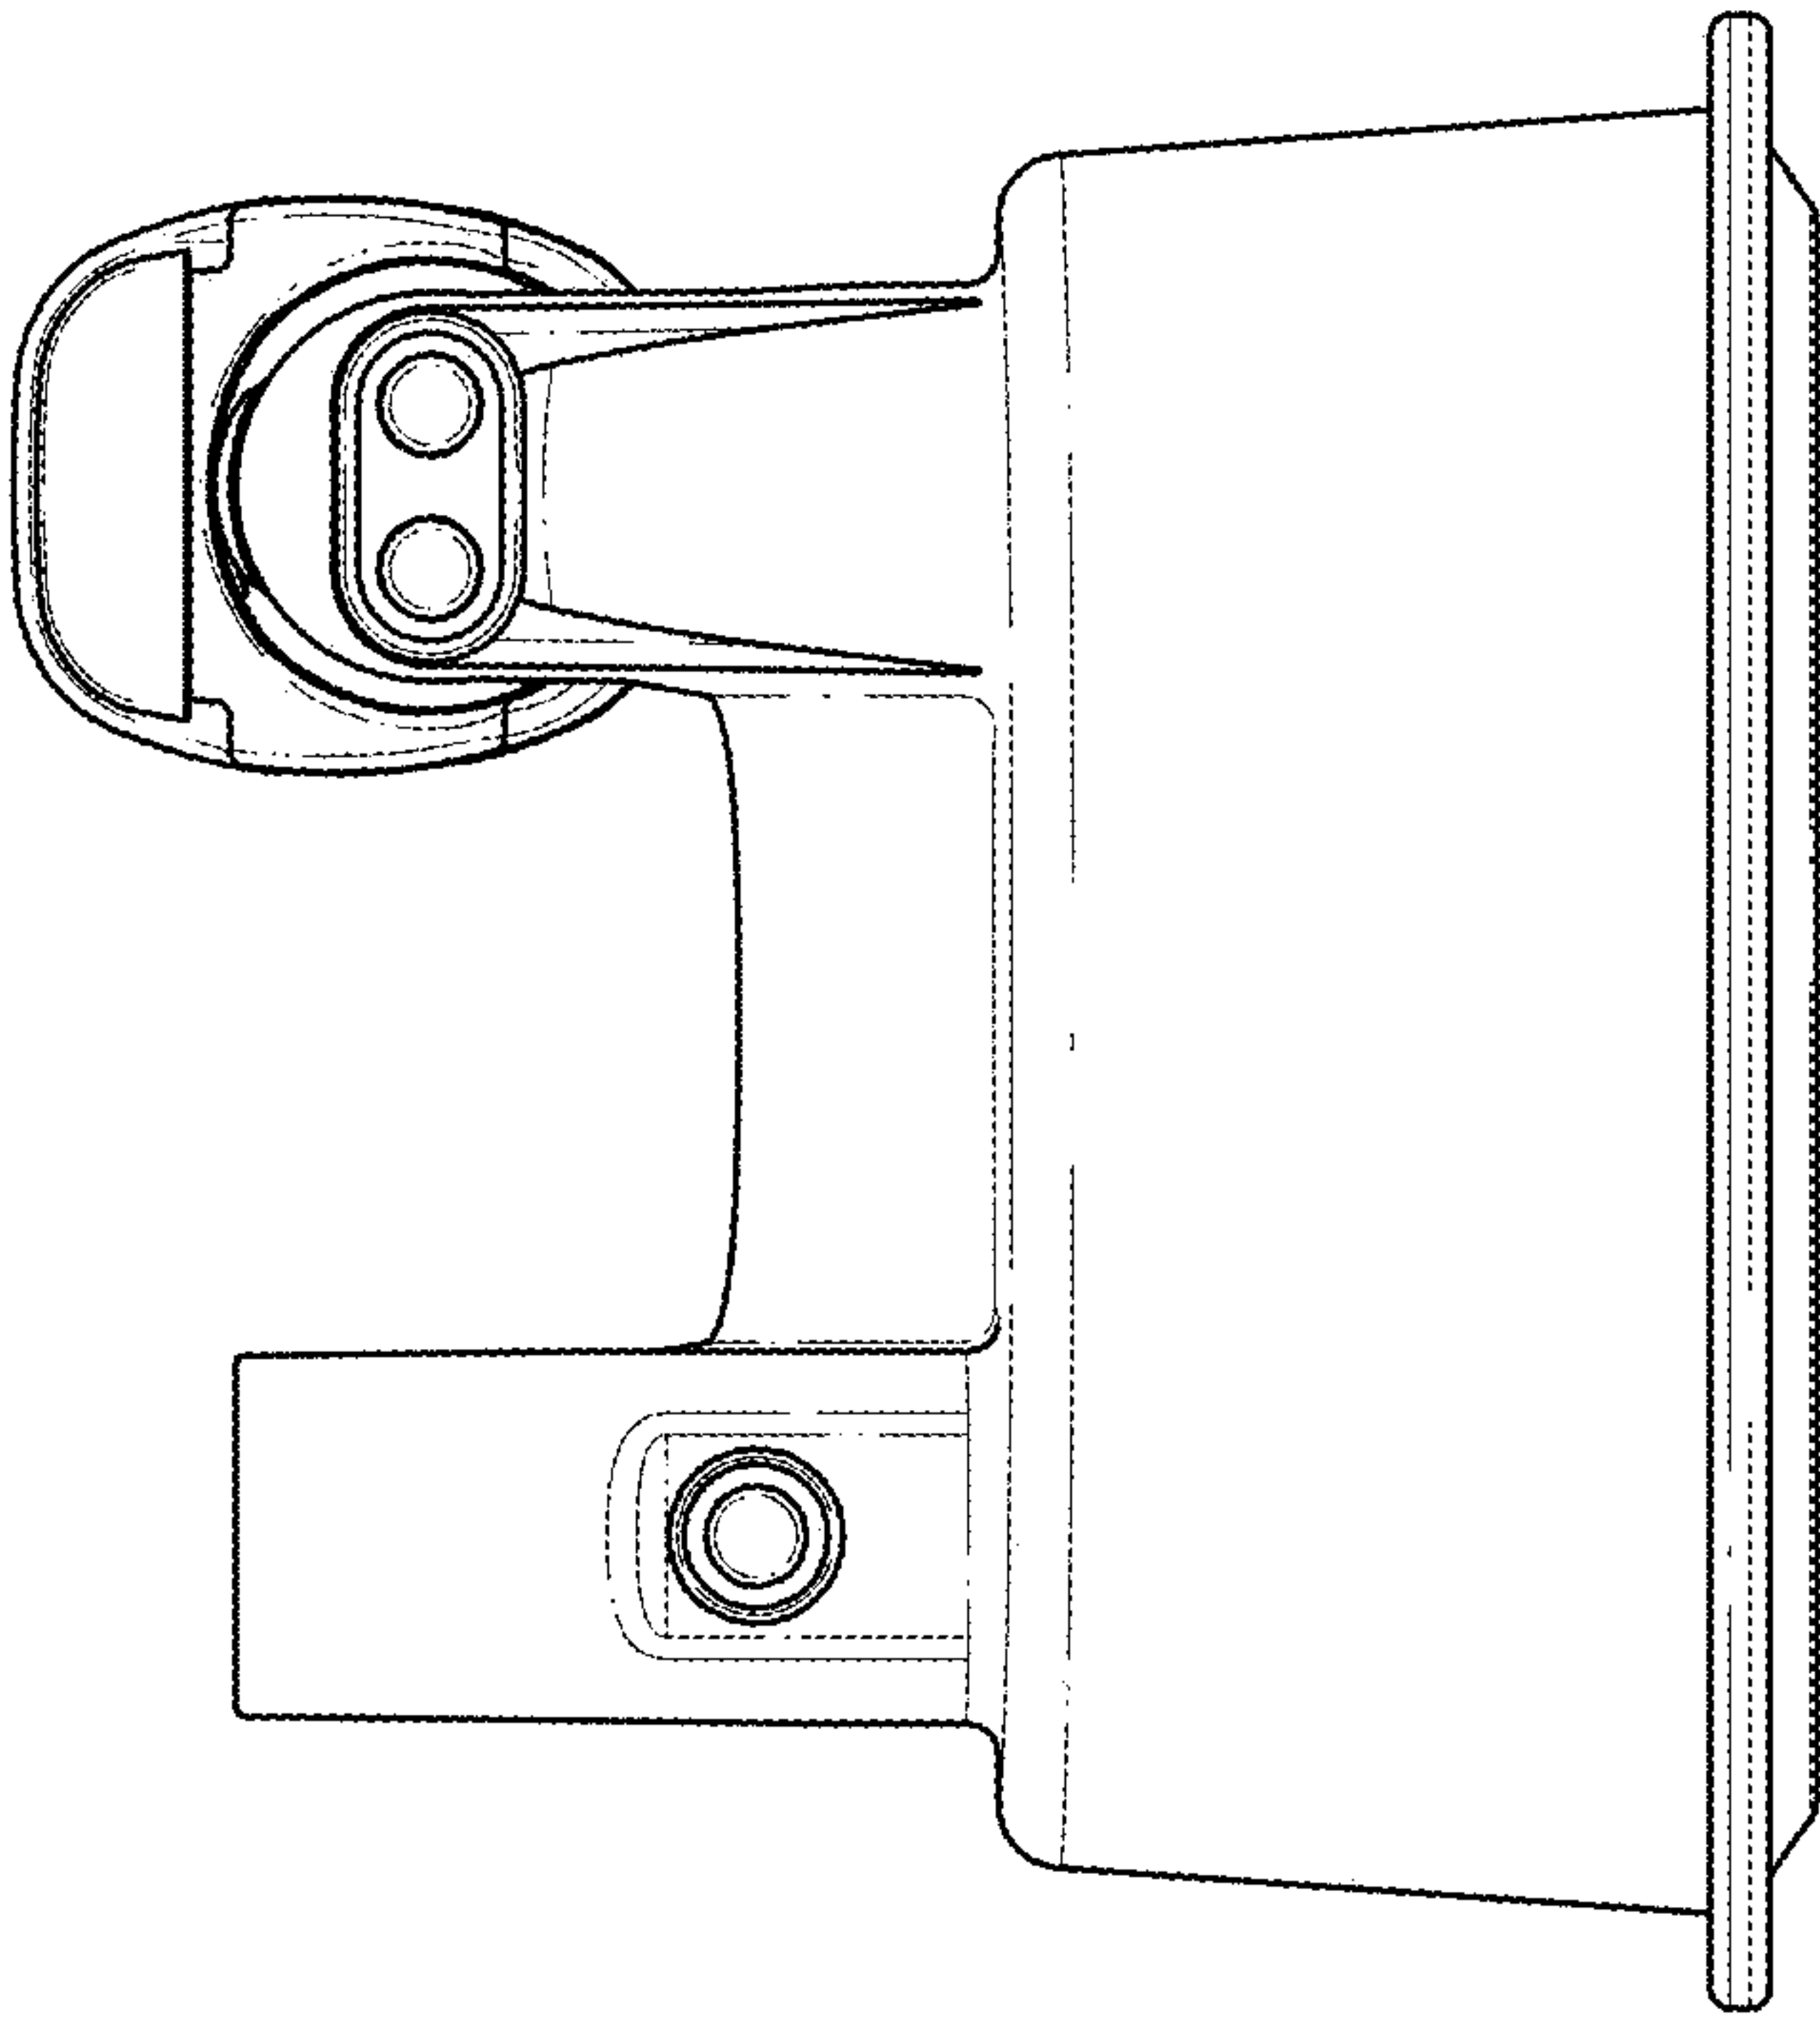


FIG. 2

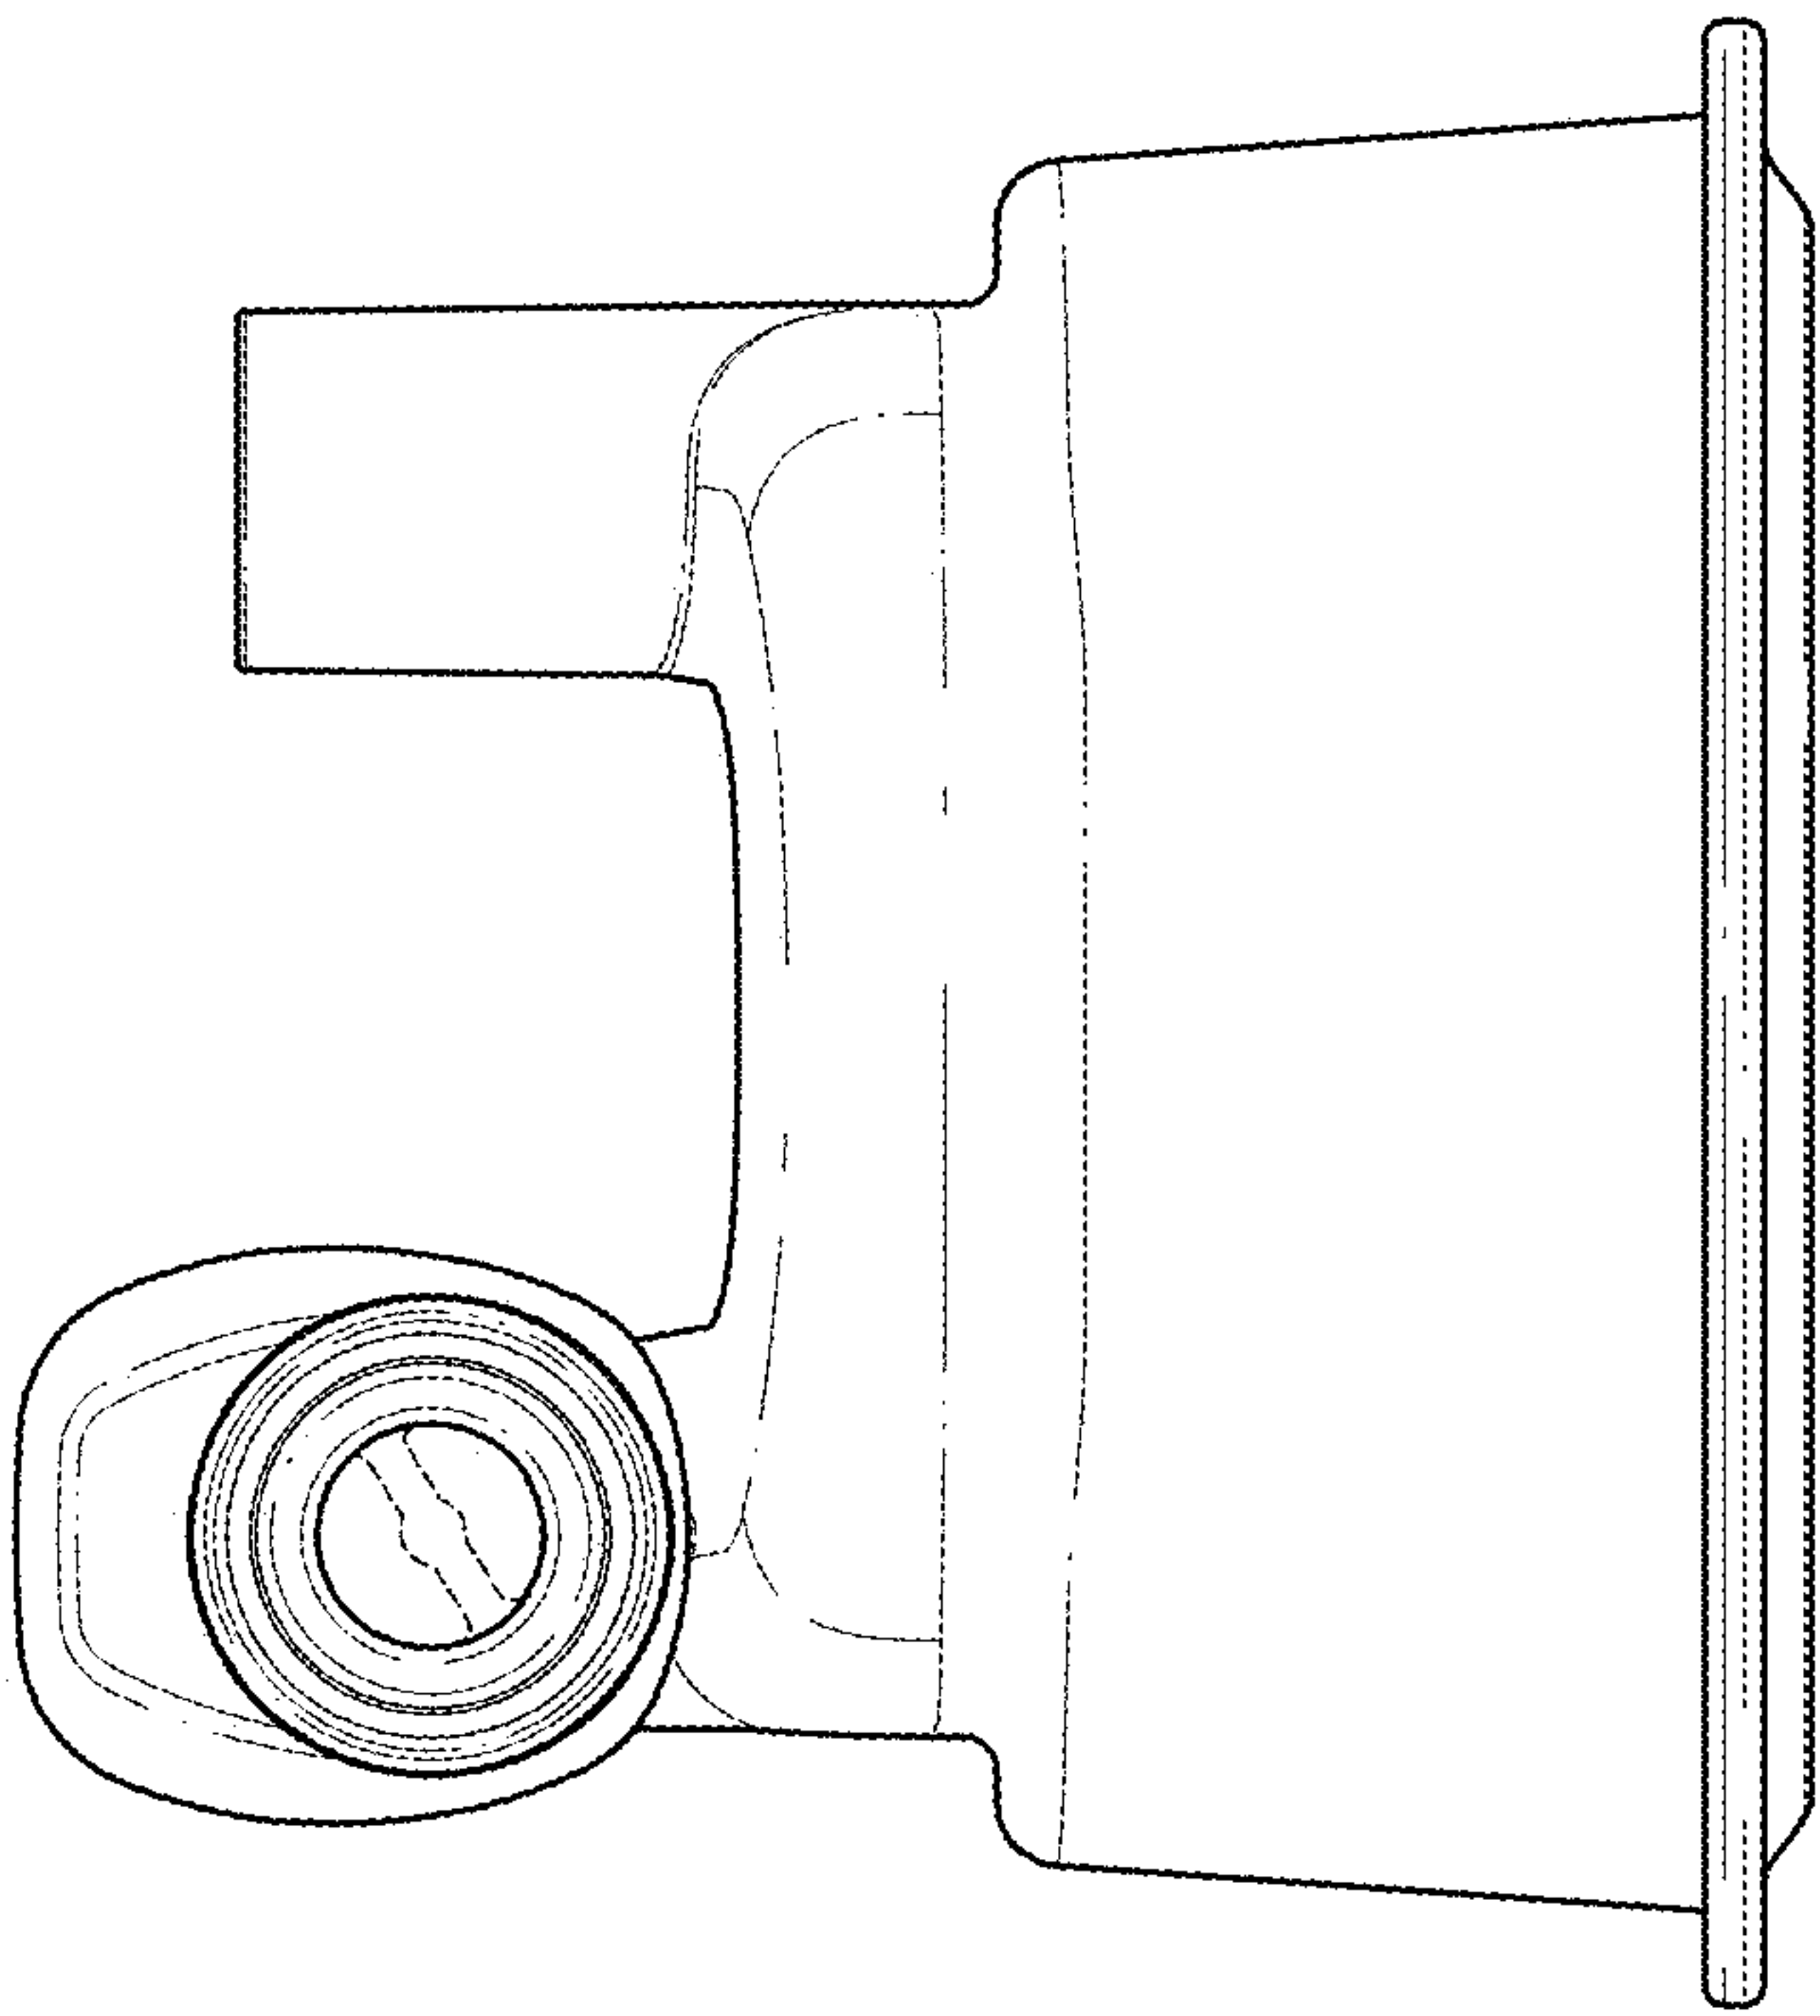


FIG.3

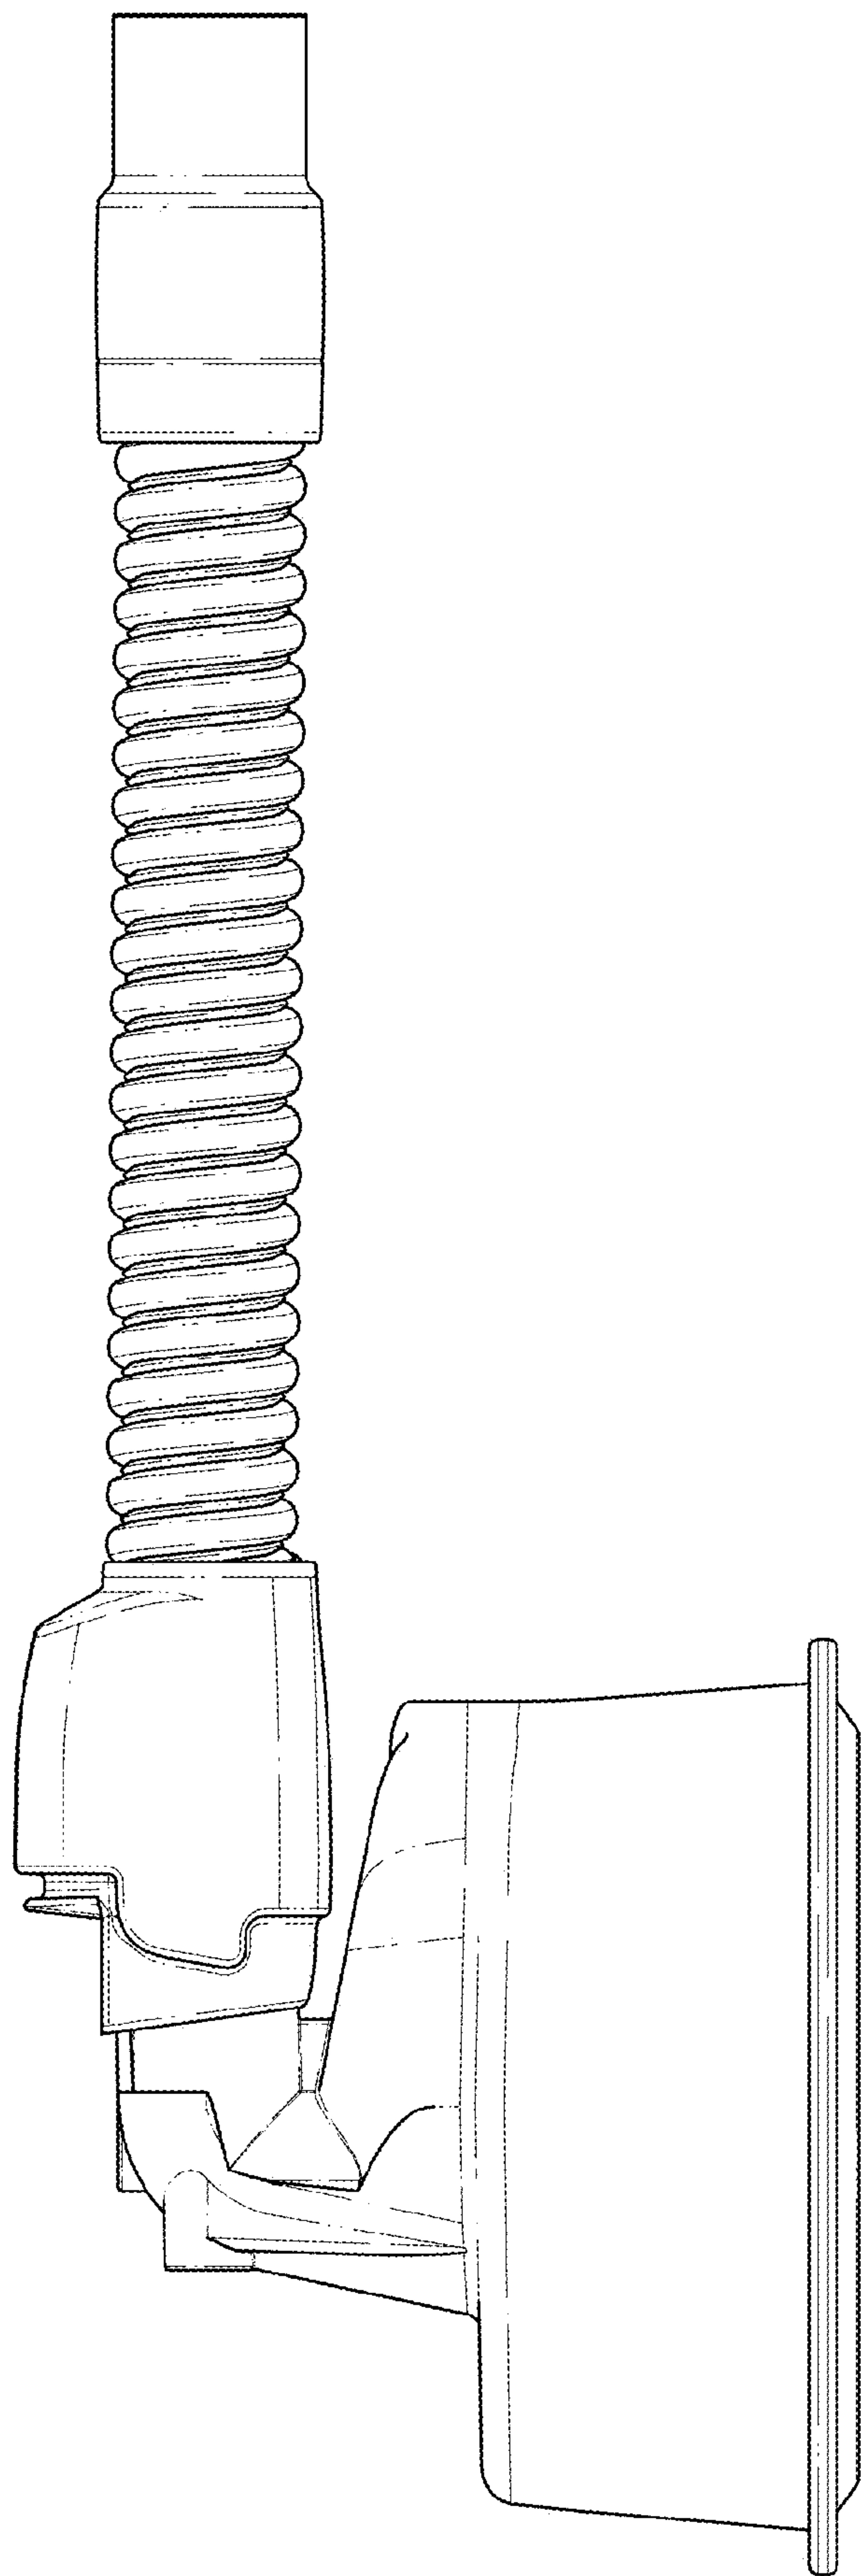


FIG.4

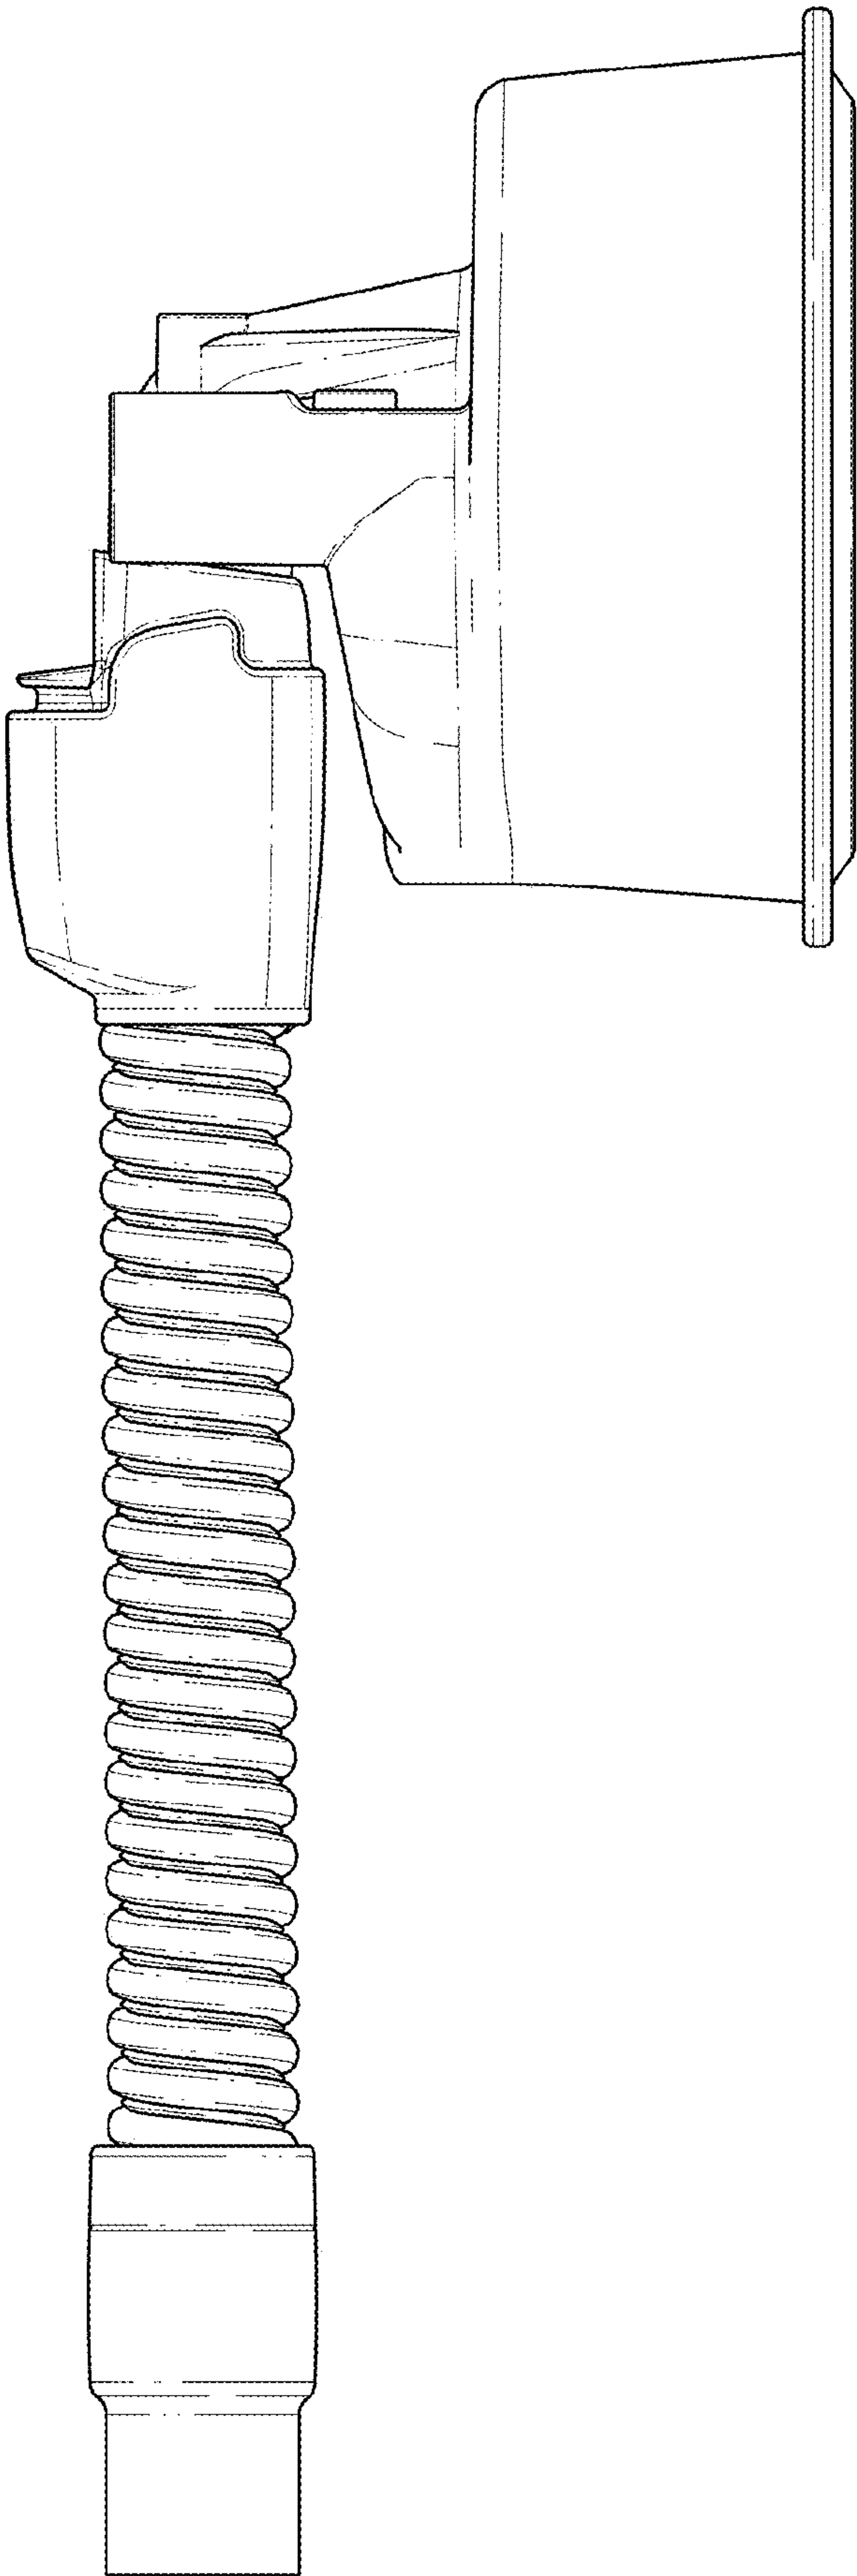


FIG.5

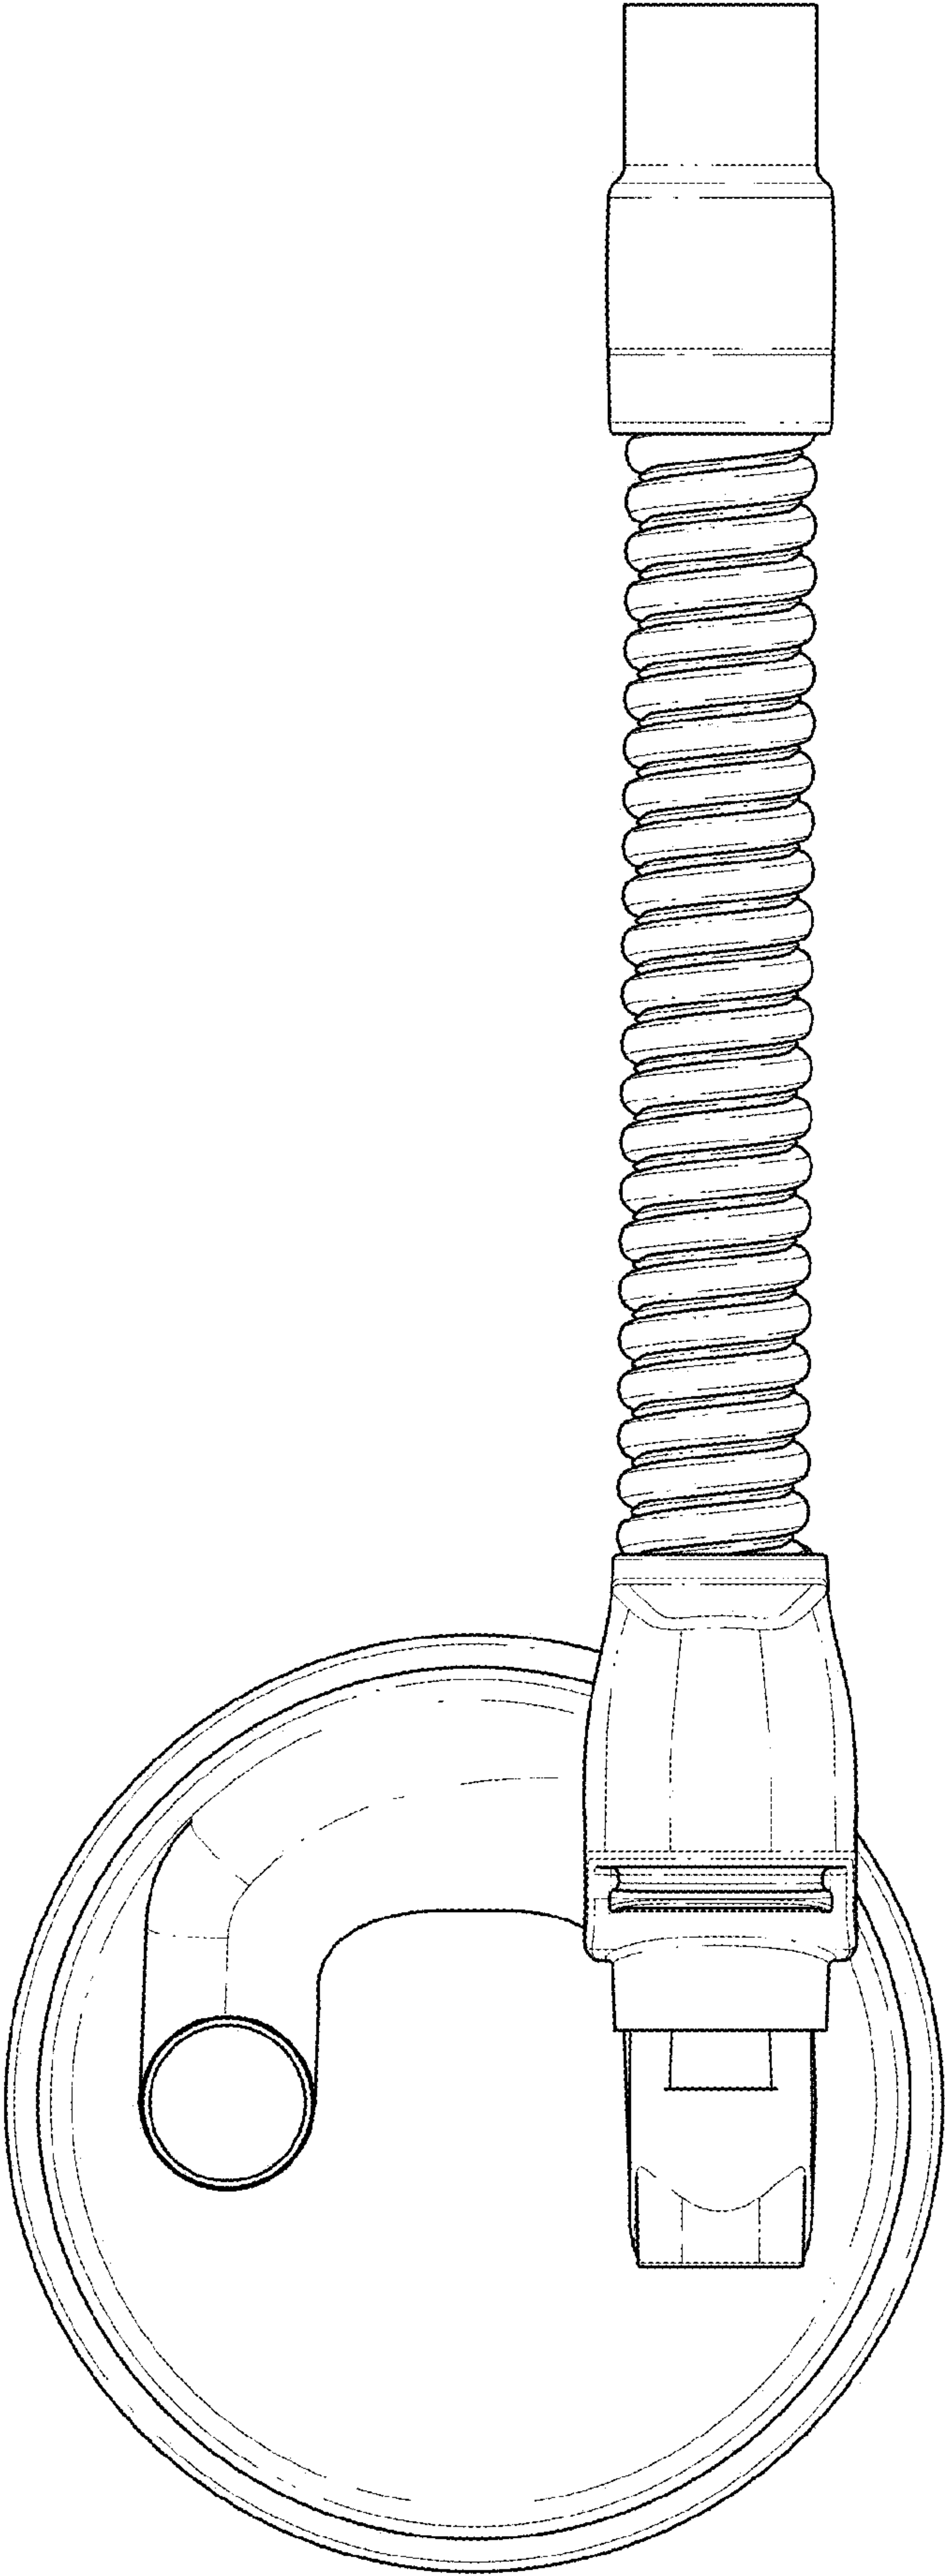


FIG.6

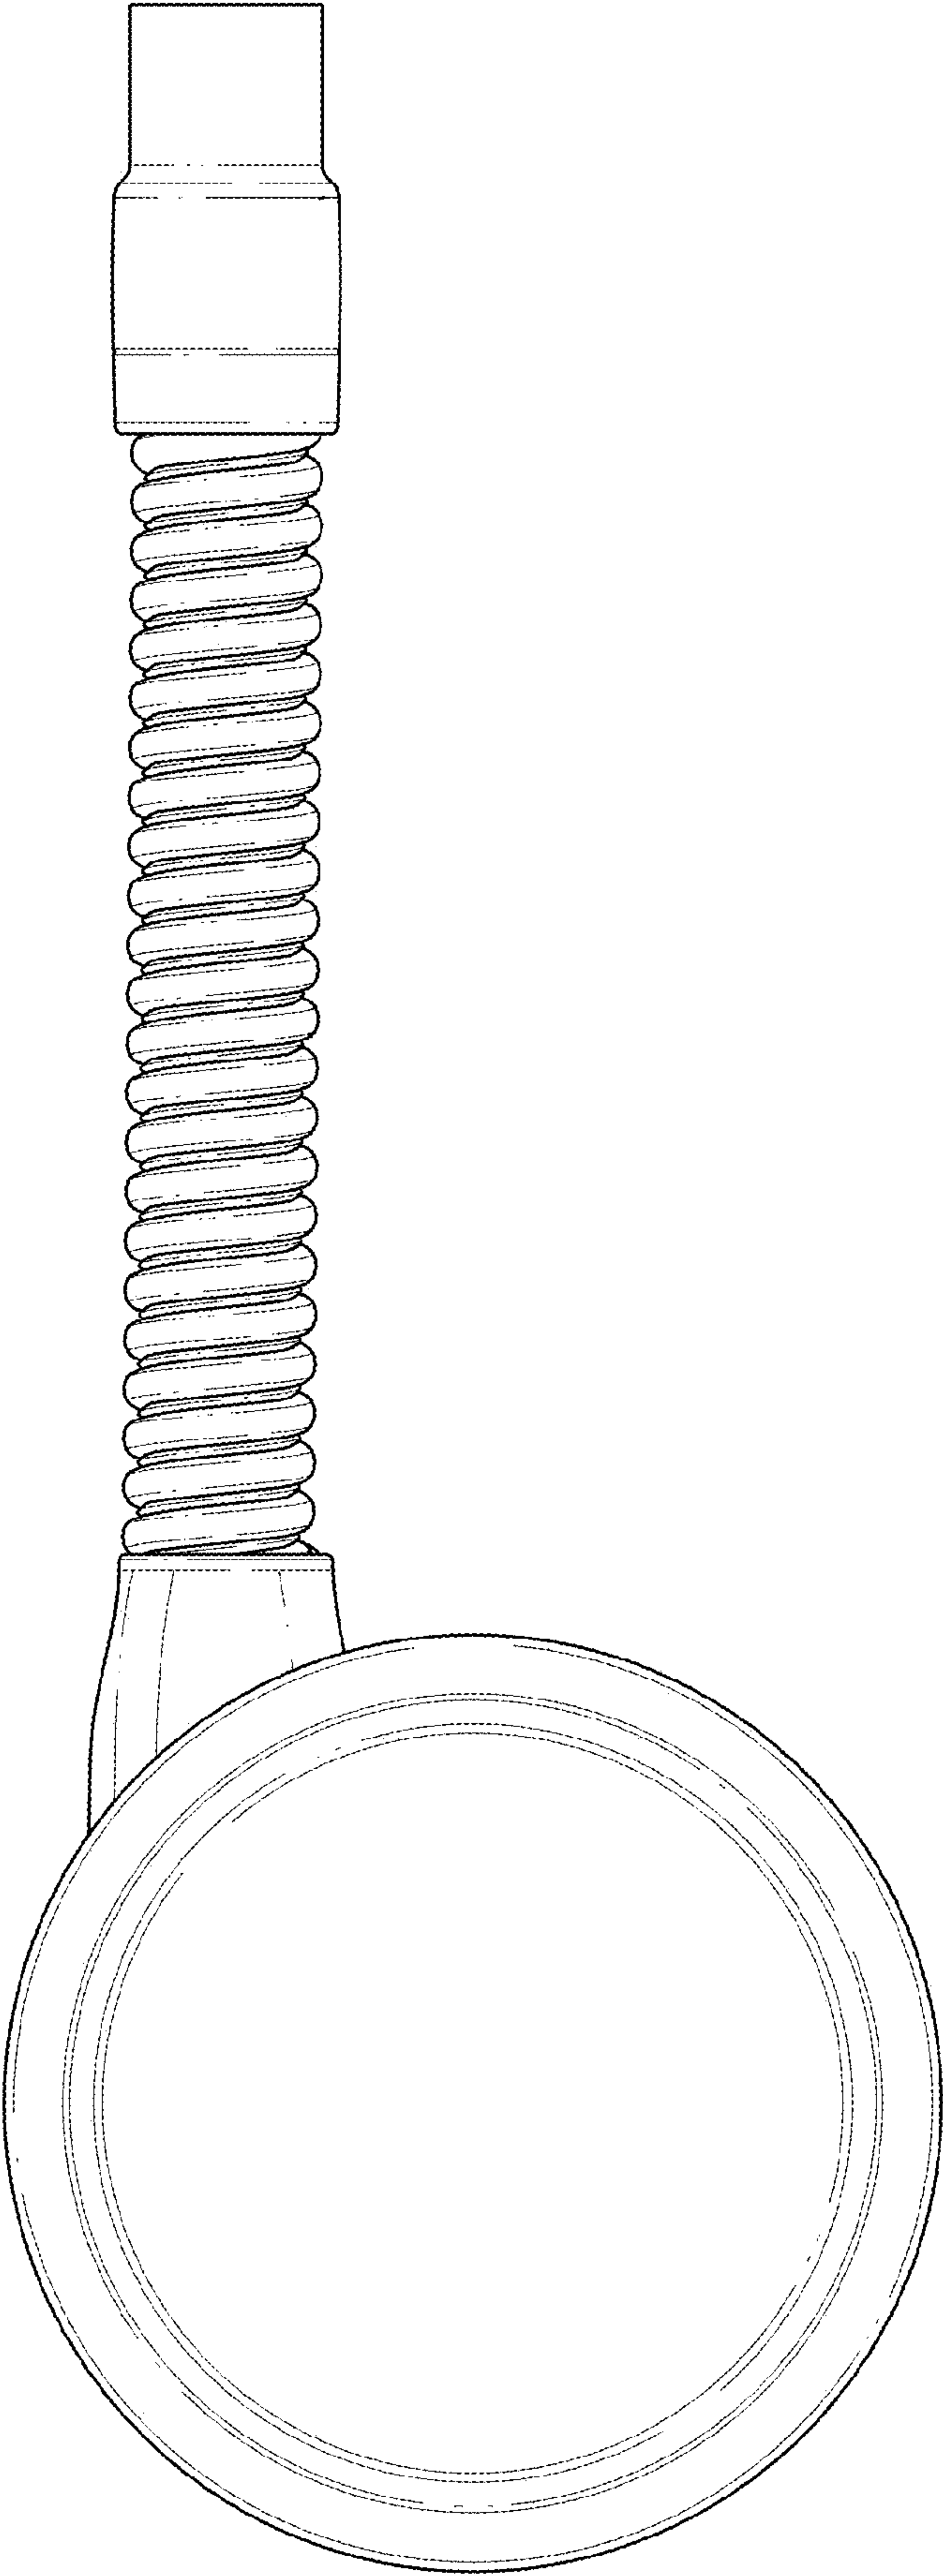


FIG.7