



US0D1008700S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,008,700 S**  
**Shanker** (45) **Date of Patent:** **\*\* Dec. 26, 2023**

(54) **NECK THERAPY CUSHION**  
(71) Applicant: **Jonathan A. Shanker**, Clayton, MO (US)  
(72) Inventor: **Jonathan A. Shanker**, Clayton, MO (US)  
(73) Assignee: **Jonathan A. Shanker**, Clayton, MO (US)

5,501,646 A 3/1996 Miller  
6,016,807 A 1/2000 Lodge  
7,347,834 B2 3/2008 Han  
8,874,227 B2 10/2014 Simon et al.  
9,004,917 B2 4/2015 Brunner  
(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 209734485 U 12/2019  
EP 2110159 B1 1/2013  
(Continued)

(\*\*) Term: **15 Years**

**OTHER PUBLICATIONS**

(21) Appl. No.: **29/788,005**  
(22) Filed: **Feb. 8, 2021**  
(51) **LOC (14) Cl.** ..... **06-13**  
(52) **U.S. Cl.**  
USPC ..... **D6/601**  
(58) **Field of Classification Search**  
USPC ..... D6/595-601, 604, 606; D24/183, 190;  
D21/803, 809  
CPC .... A47A 20/00; A47A 20/021; A47D 15/001;  
A47D 15/008; A47G 9/00; A47G 9/10;  
A47C 7/742; A47C 7/021; A47C 27/00;  
B62J 1/26  
See application file for complete search history.

Larkin-Kaiser et al., "Near-Infrared Light Therapy to Attenuate Strength Loss After Strenuous Resistance Exercise," NATA Journals, 2015, vol. 50, No. 1, retrieved from <https://ncbi.nlm.nih.gov/pmc/articles/PMC4299734/> on Feb. 7, 2020, pp. 45-50.

(Continued)

*Primary Examiner* — Cynthia Ramirez  
*Assistant Examiner* — Carrie A Matteoli  
(74) *Attorney, Agent, or Firm* — Armstrong Teasdale LLP

(57) **CLAIM**

I claim the ornamental design for a neck therapy cushion, as shown and described.

(56) **References Cited**


**DESCRIPTION**

**U.S. PATENT DOCUMENTS**

1,890,358 A \* 12/1932 Barcalo ..... A47G 9/10  
5/636  
1,928,806 A \* 10/1933 Barcalo ..... A47G 9/1045  
428/6  
1,934,254 A \* 11/1933 Barcalo ..... A47G 9/1045  
5/639  
2,877,472 A \* 3/1959 Wagner ..... A47G 9/10  
5/636  
4,836,778 A 6/1989 Baumrind et al.  
D303,560 S \* 9/1989 Scheurer ..... D21/809  
5,163,194 A 11/1992 Dixon

FIG. 1 is a perspective view of a neck therapy cushion showing the new design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a rear view thereof;  
FIG. 4 is a left side view thereof;  
FIG. 5 is a right side view thereof; and,  
FIG. 6 is a top view thereof.  
The broken lines in the figures show portions of the neck therapy cushion which form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

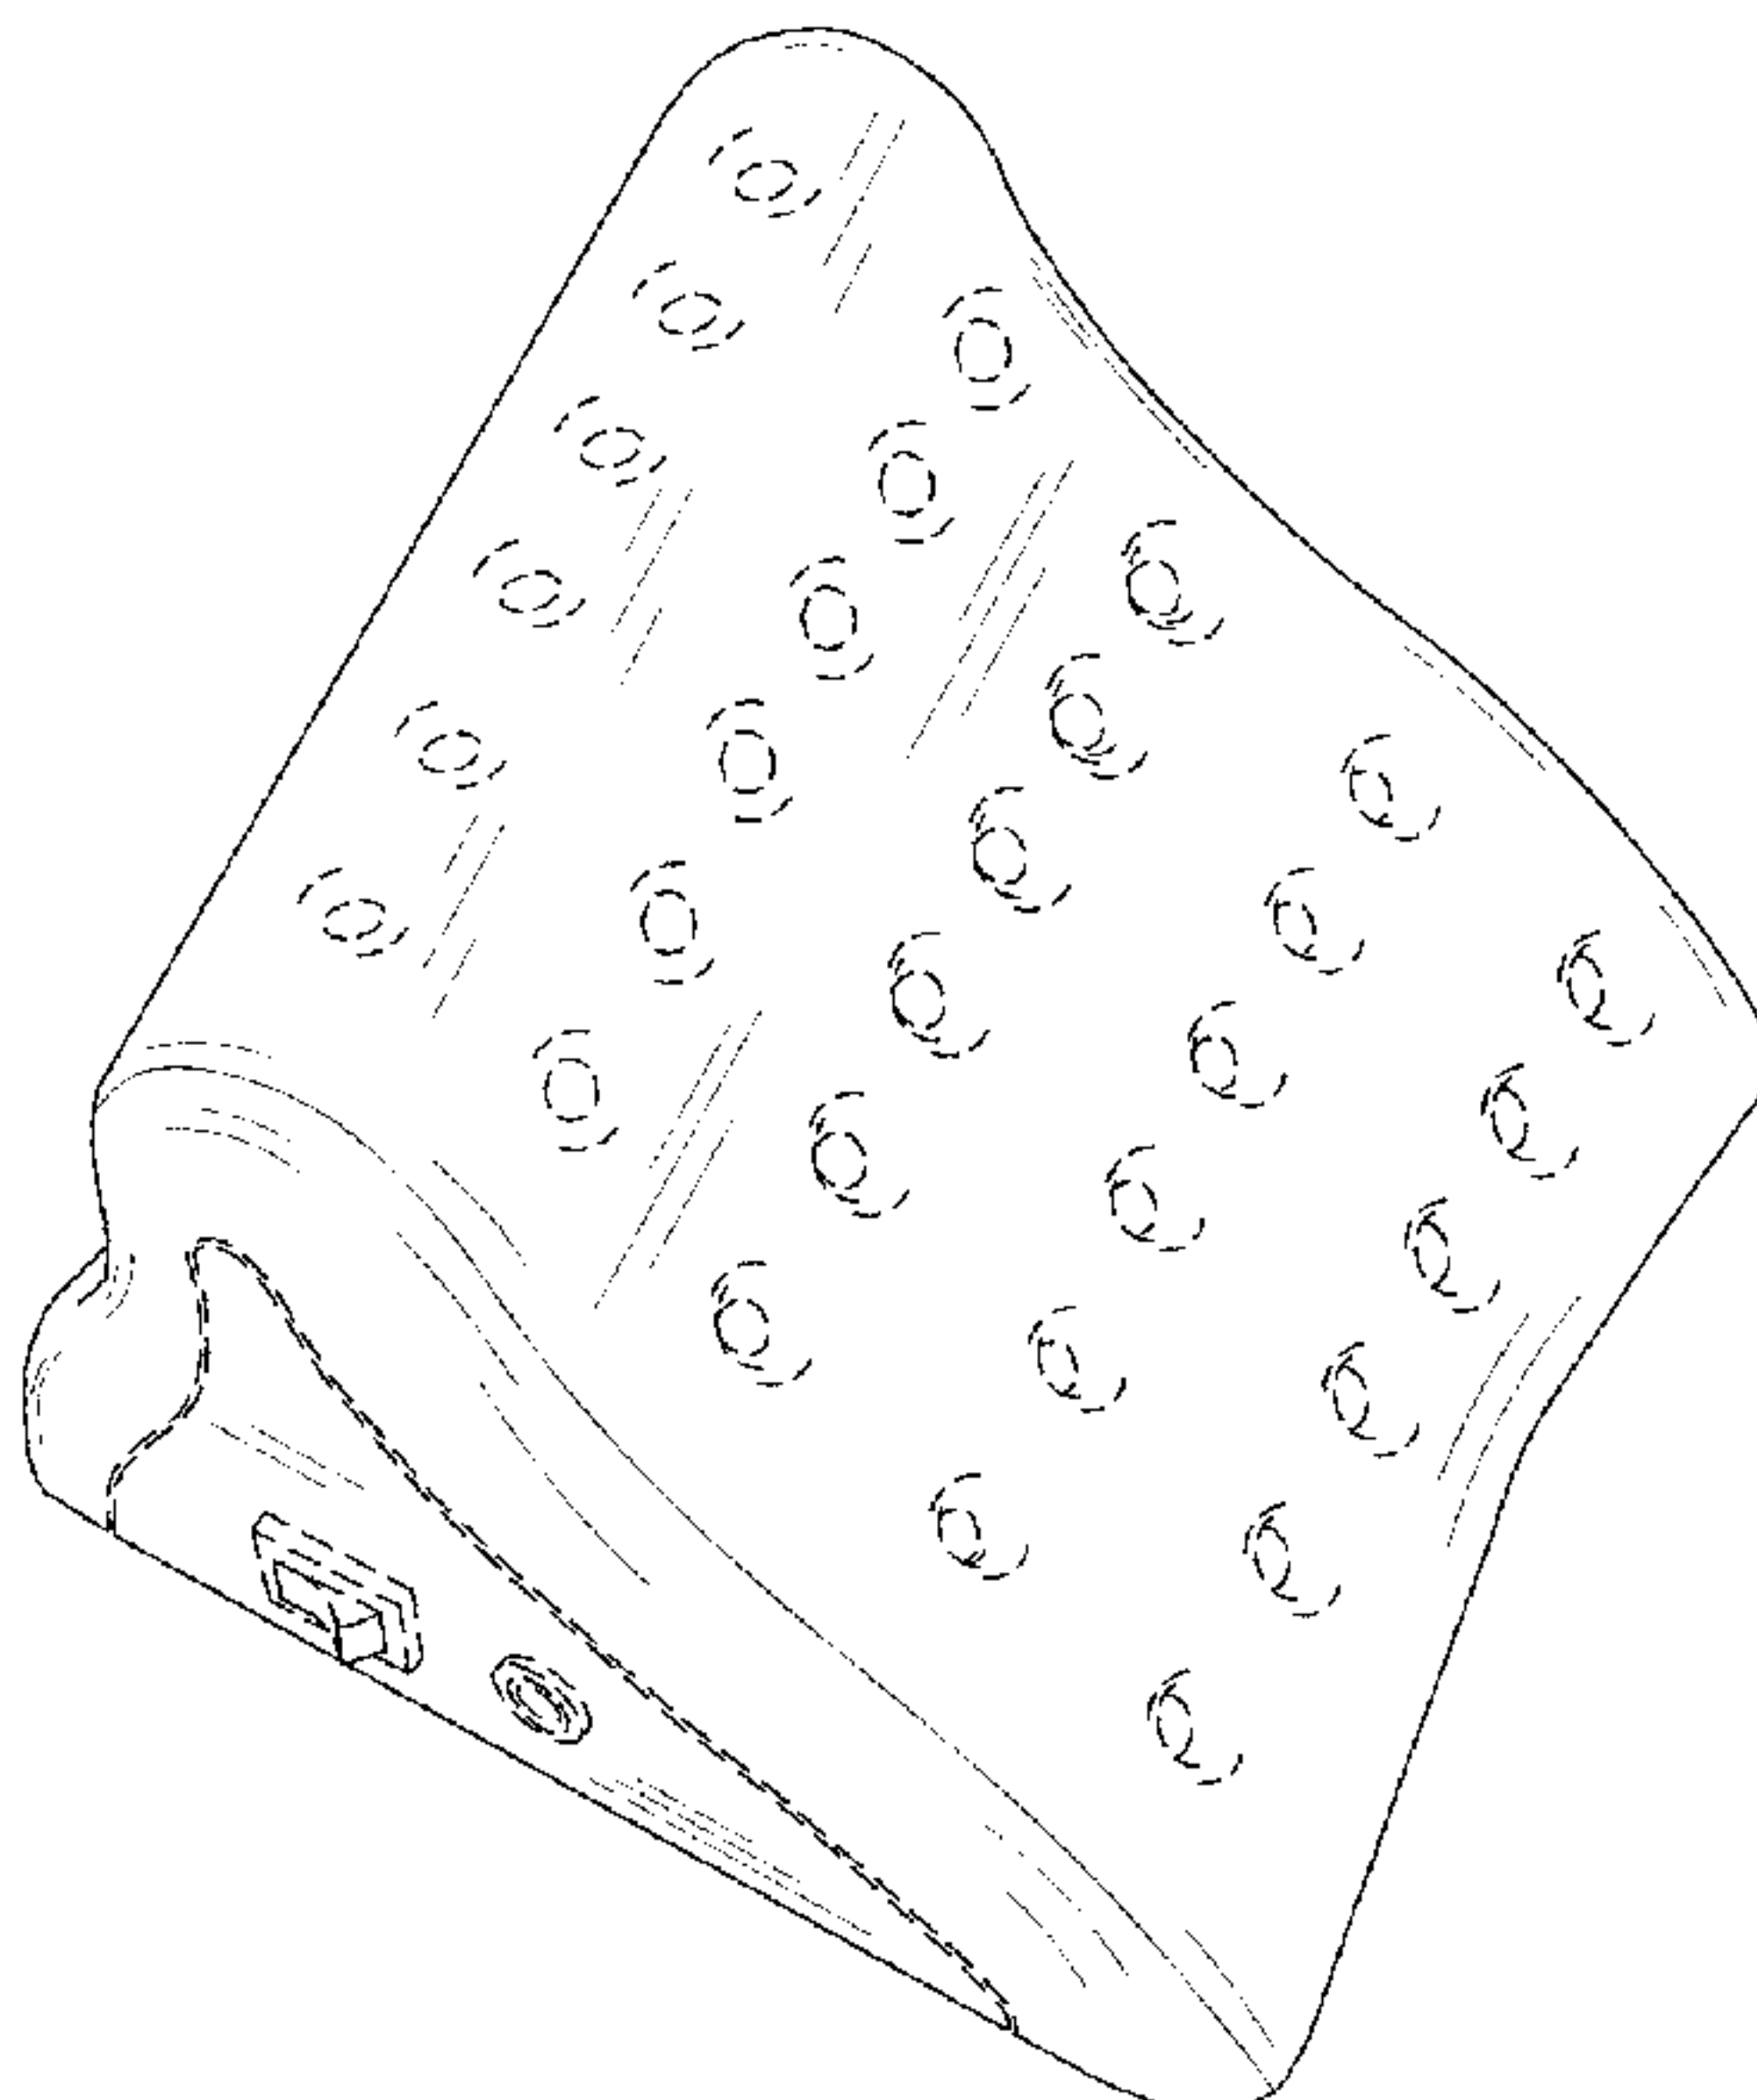

(56)

**References Cited**

U.S. PATENT DOCUMENTS

9,242,118 B2 1/2016 Brawn  
D752,899 S \* 4/2016 Ueno ..... D6/601  
D909,587 S \* 2/2021 Barcohana ..... D24/171  
2005/0278003 A1 12/2005 Feldman  
2007/0248930 A1 10/2007 Brawn  
2012/0148976 A1 6/2012 Brawn  
2017/0128307 A1 5/2017 Kim  
2017/0216617 A1 8/2017 Kariguddaiah  
2018/0042409 A1 2/2018 Johnson  
2018/0063612 A1 3/2018 Fuchs et al.  
2019/0083809 A1 3/2019 Zhang  
2019/0143114 A1 5/2019 Nelson  
2019/0366115 A1 12/2019 Castel

FOREIGN PATENT DOCUMENTS

WO 2006059889 A1 6/2006  
WO 2019173167 A1 9/2019

OTHER PUBLICATIONS

Foley, Kevin T., et al., Randomized, prospective, and controlled clinical trial of pulsed electromagnetic field stimulation for cervical fusion, *The Spine Journal*, 2008, pp. 436-442, No. 8, Elsevier Inc. International Search Report and Written Opinion, dated Jul. 23, 2021, for related International Application No. PCT/US2021/017205 (15 pgs.).

\* cited by examiner

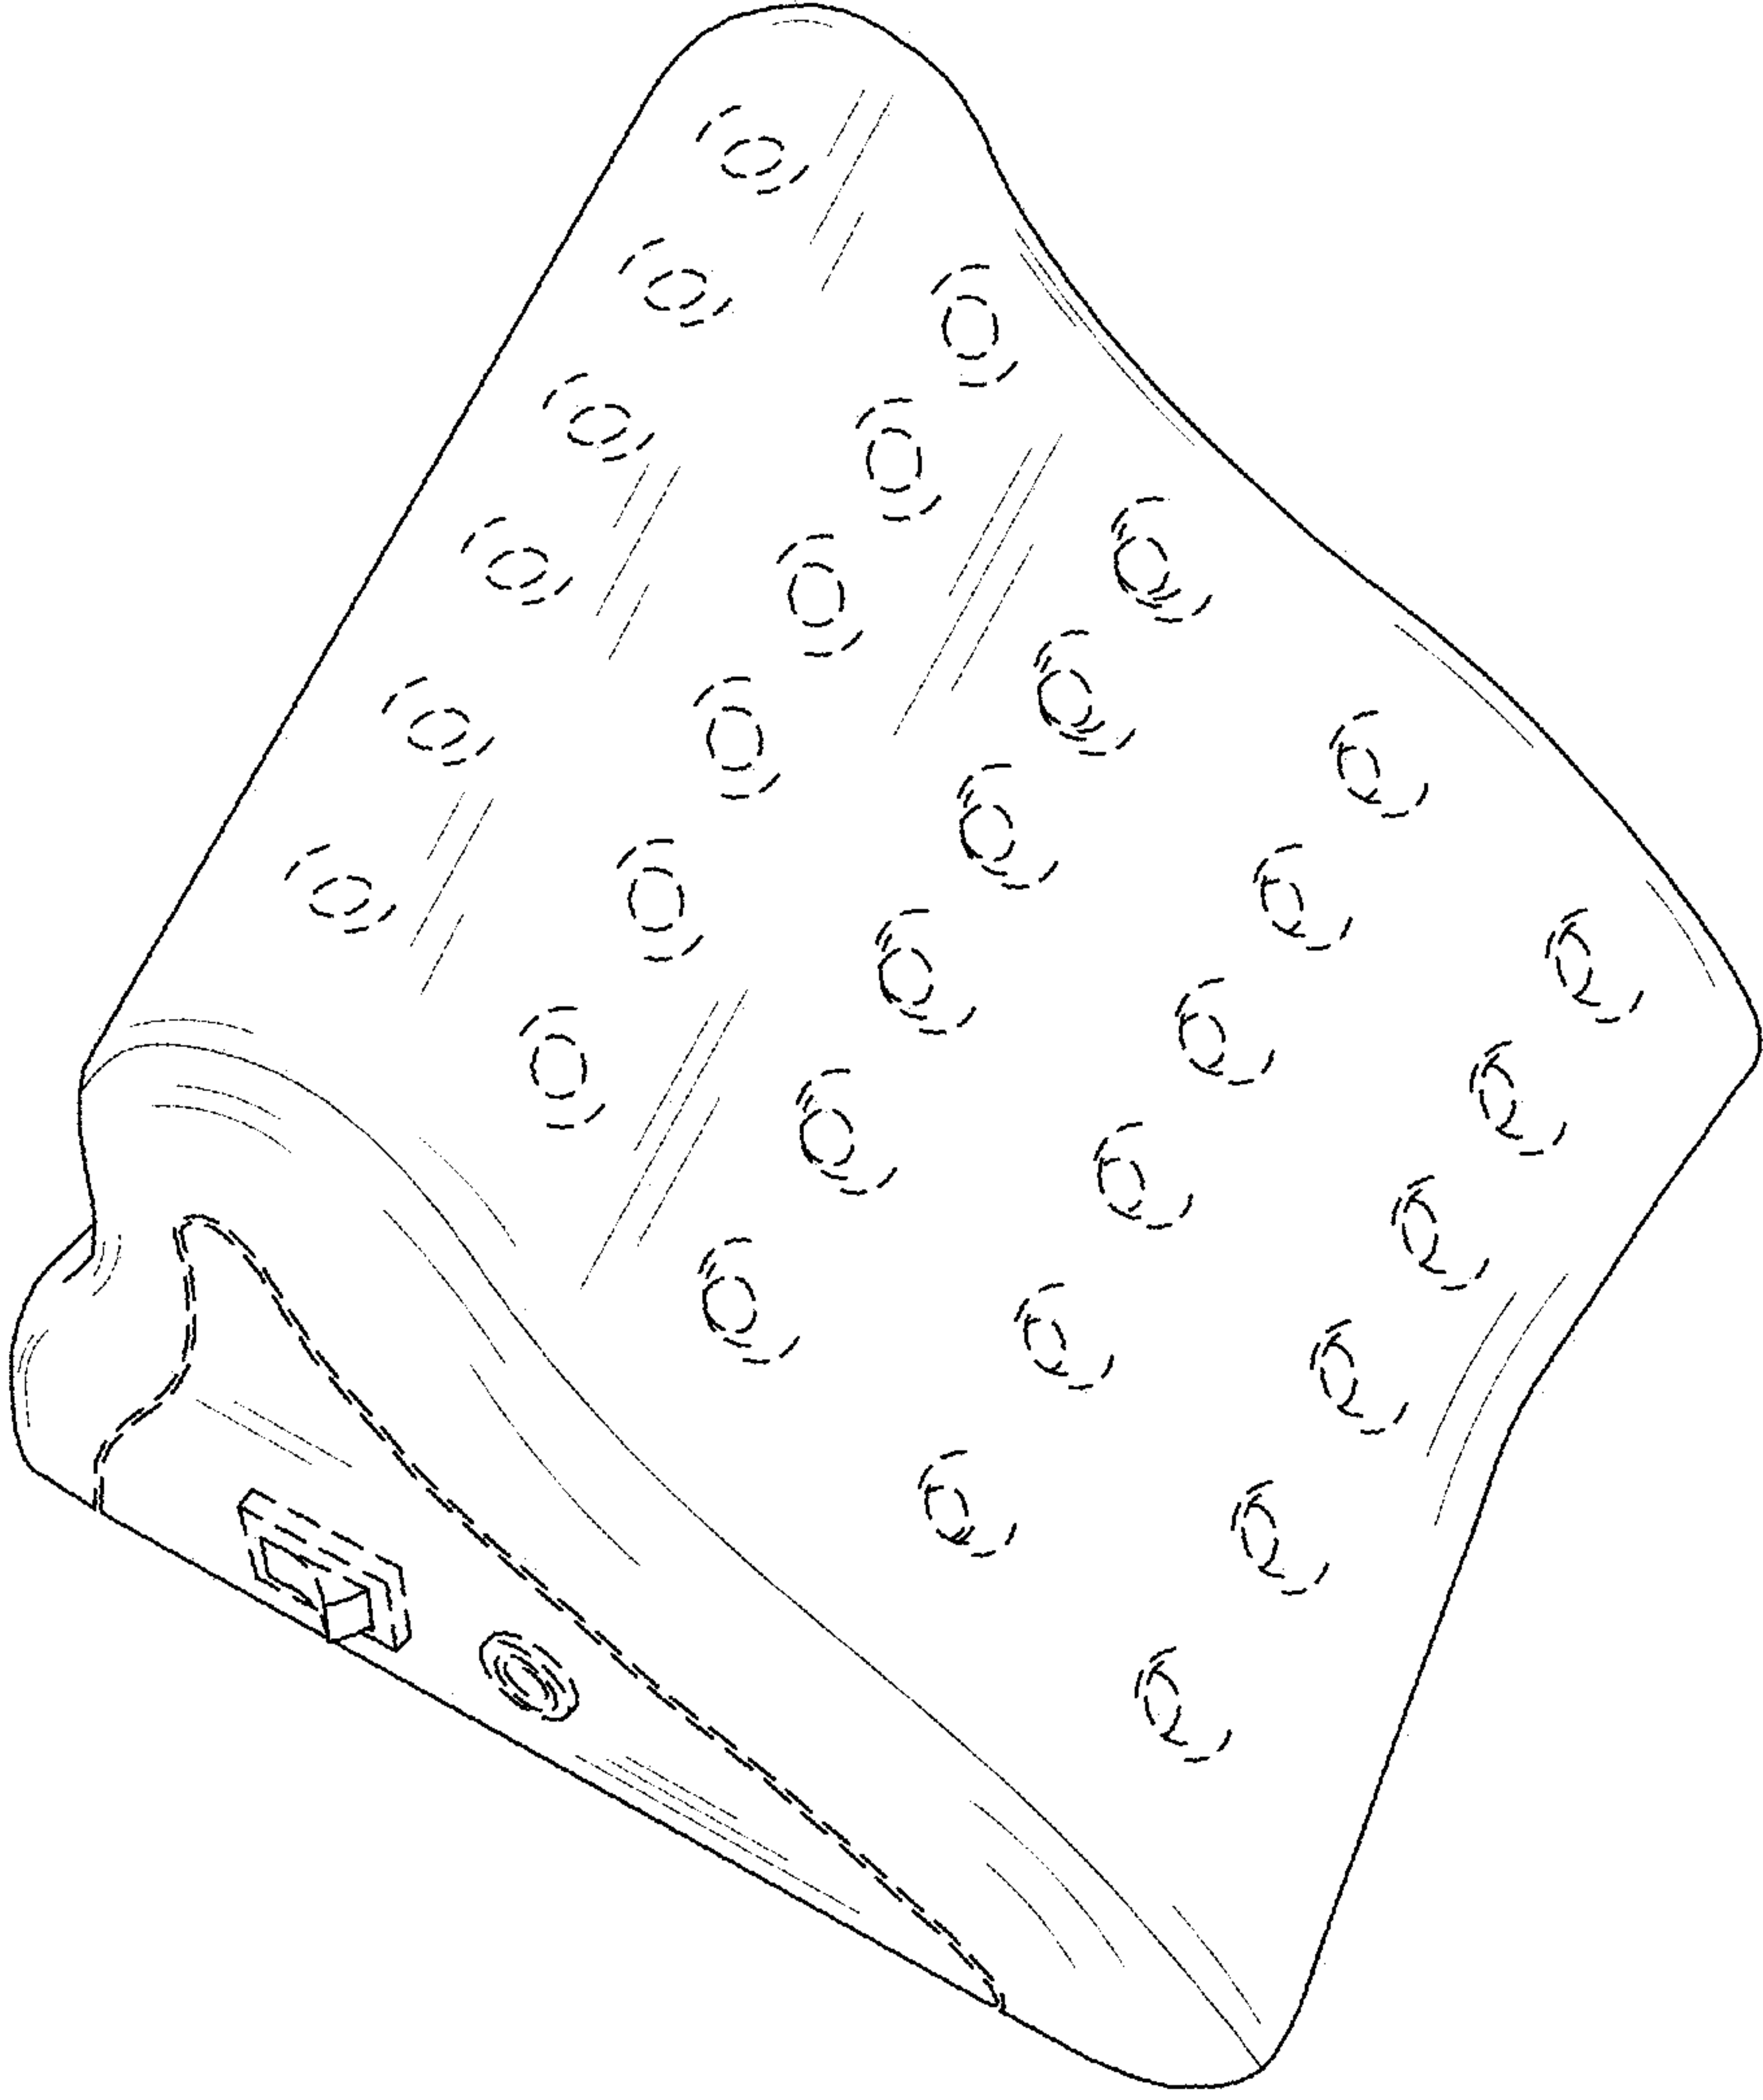


FIG. 1

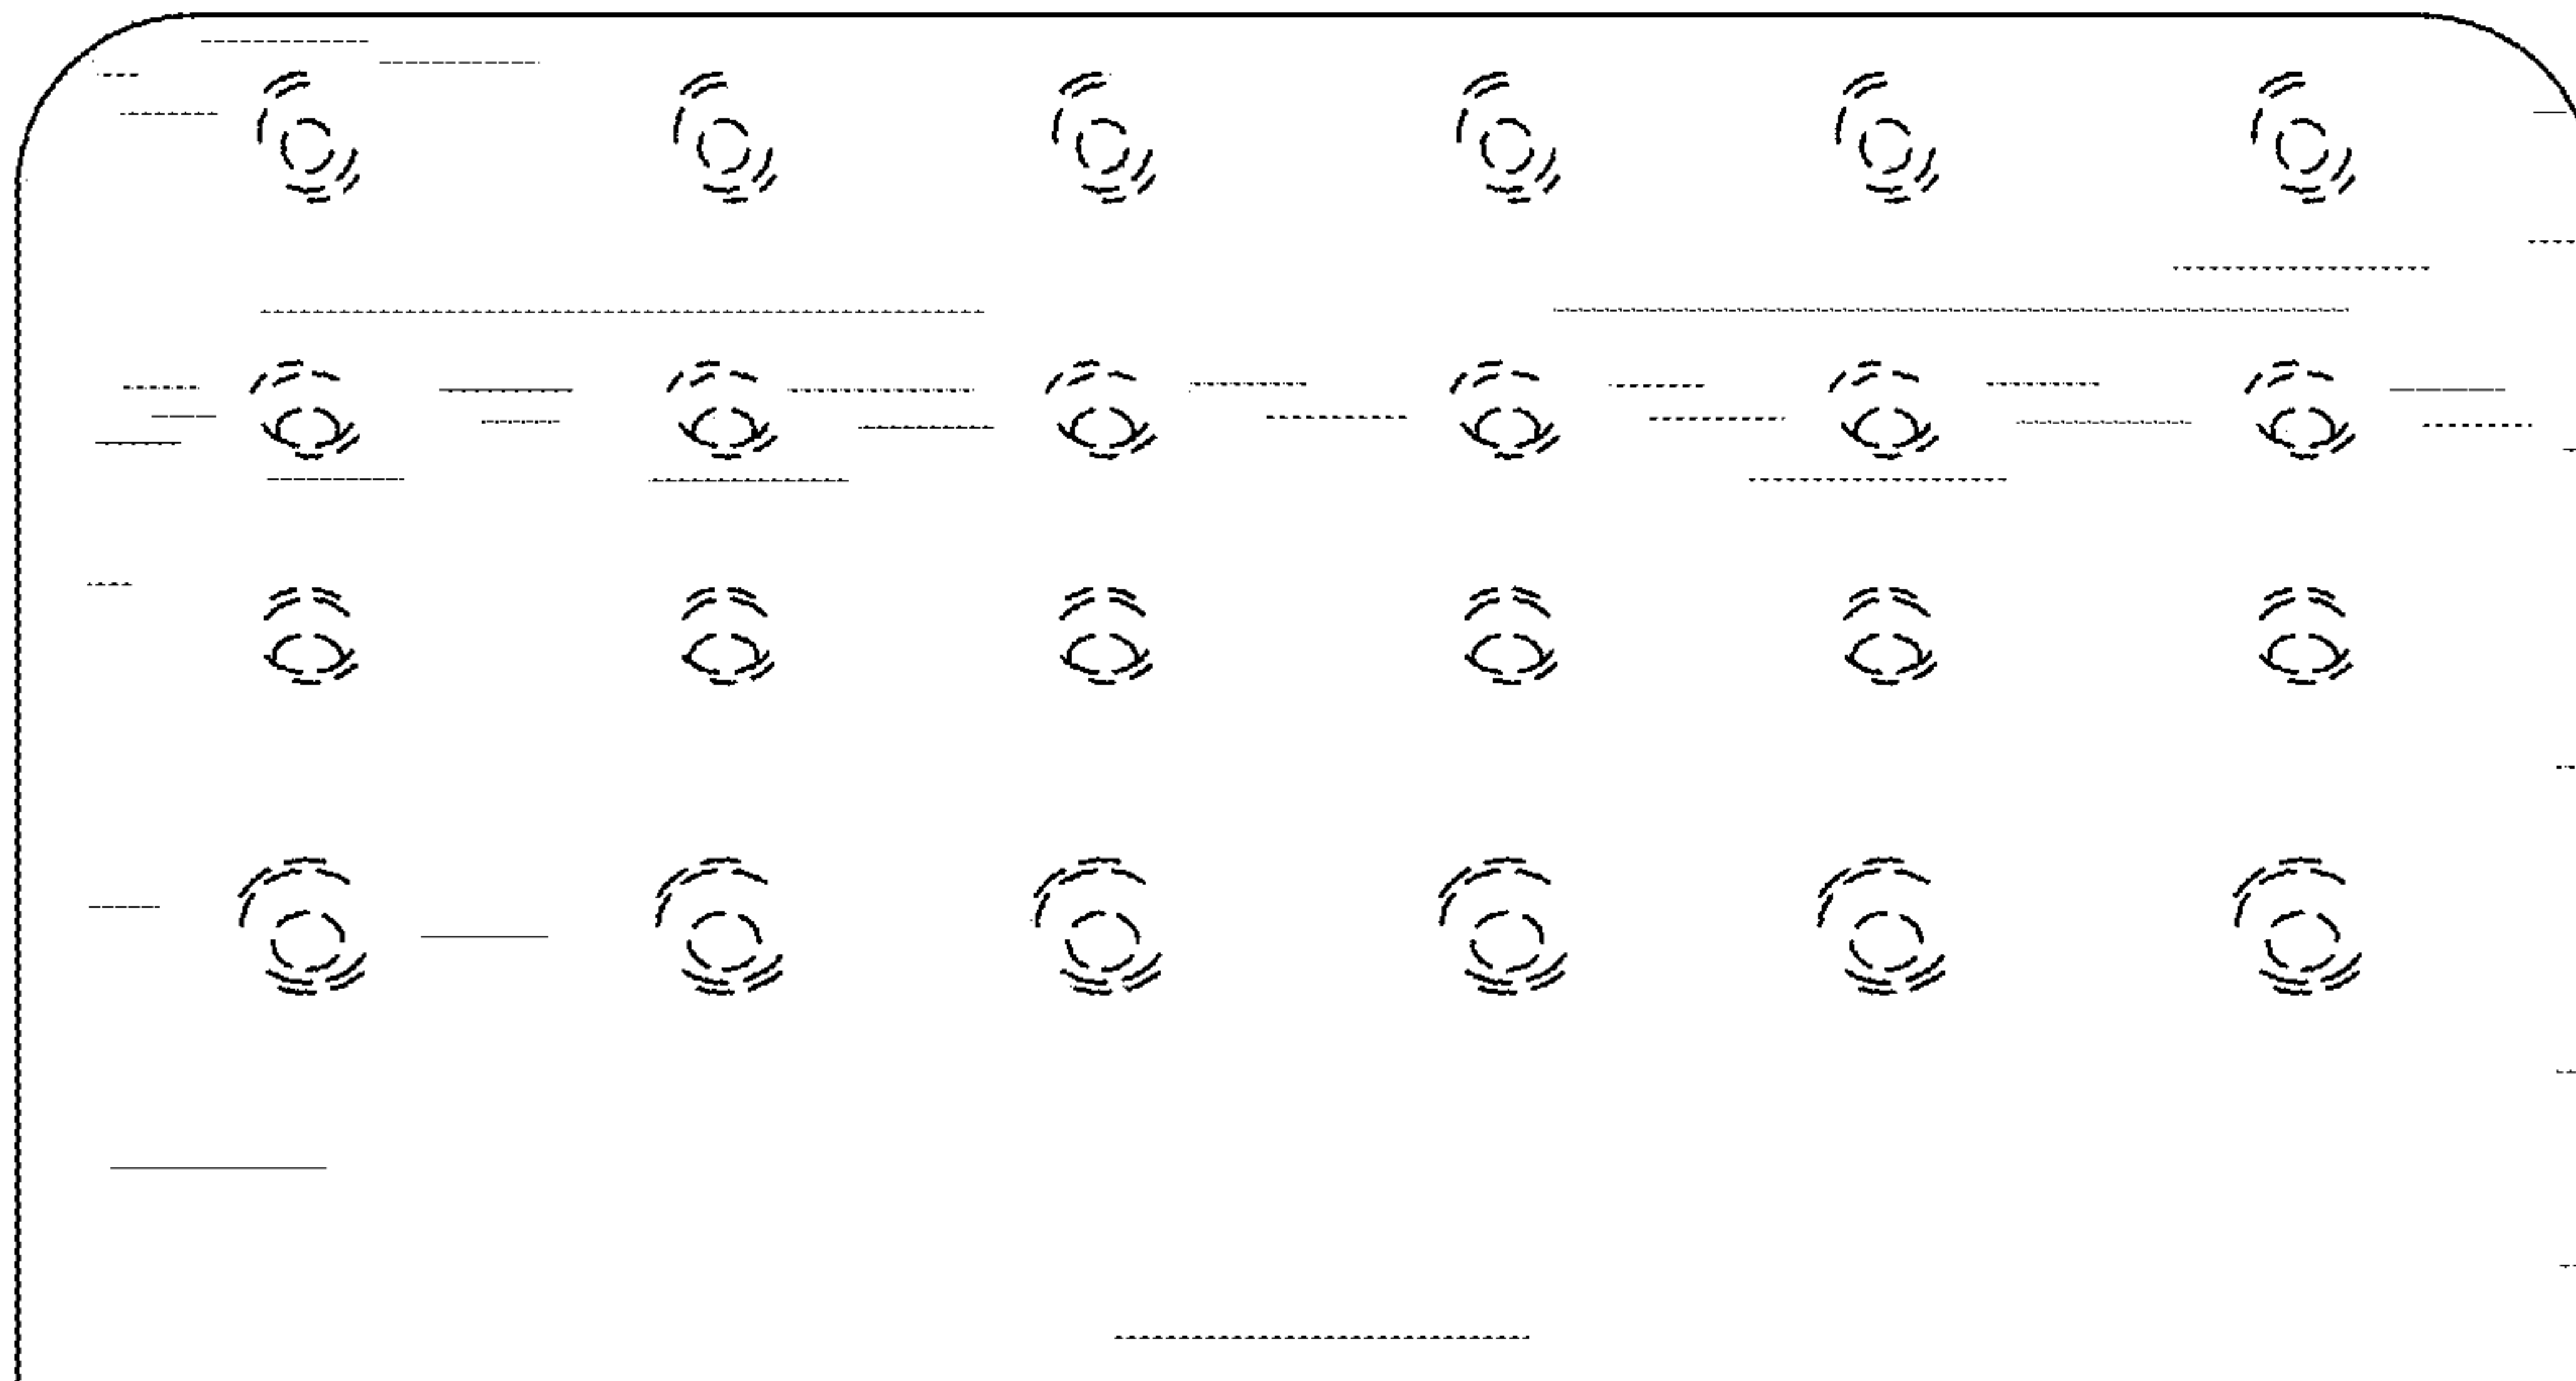


FIG. 2

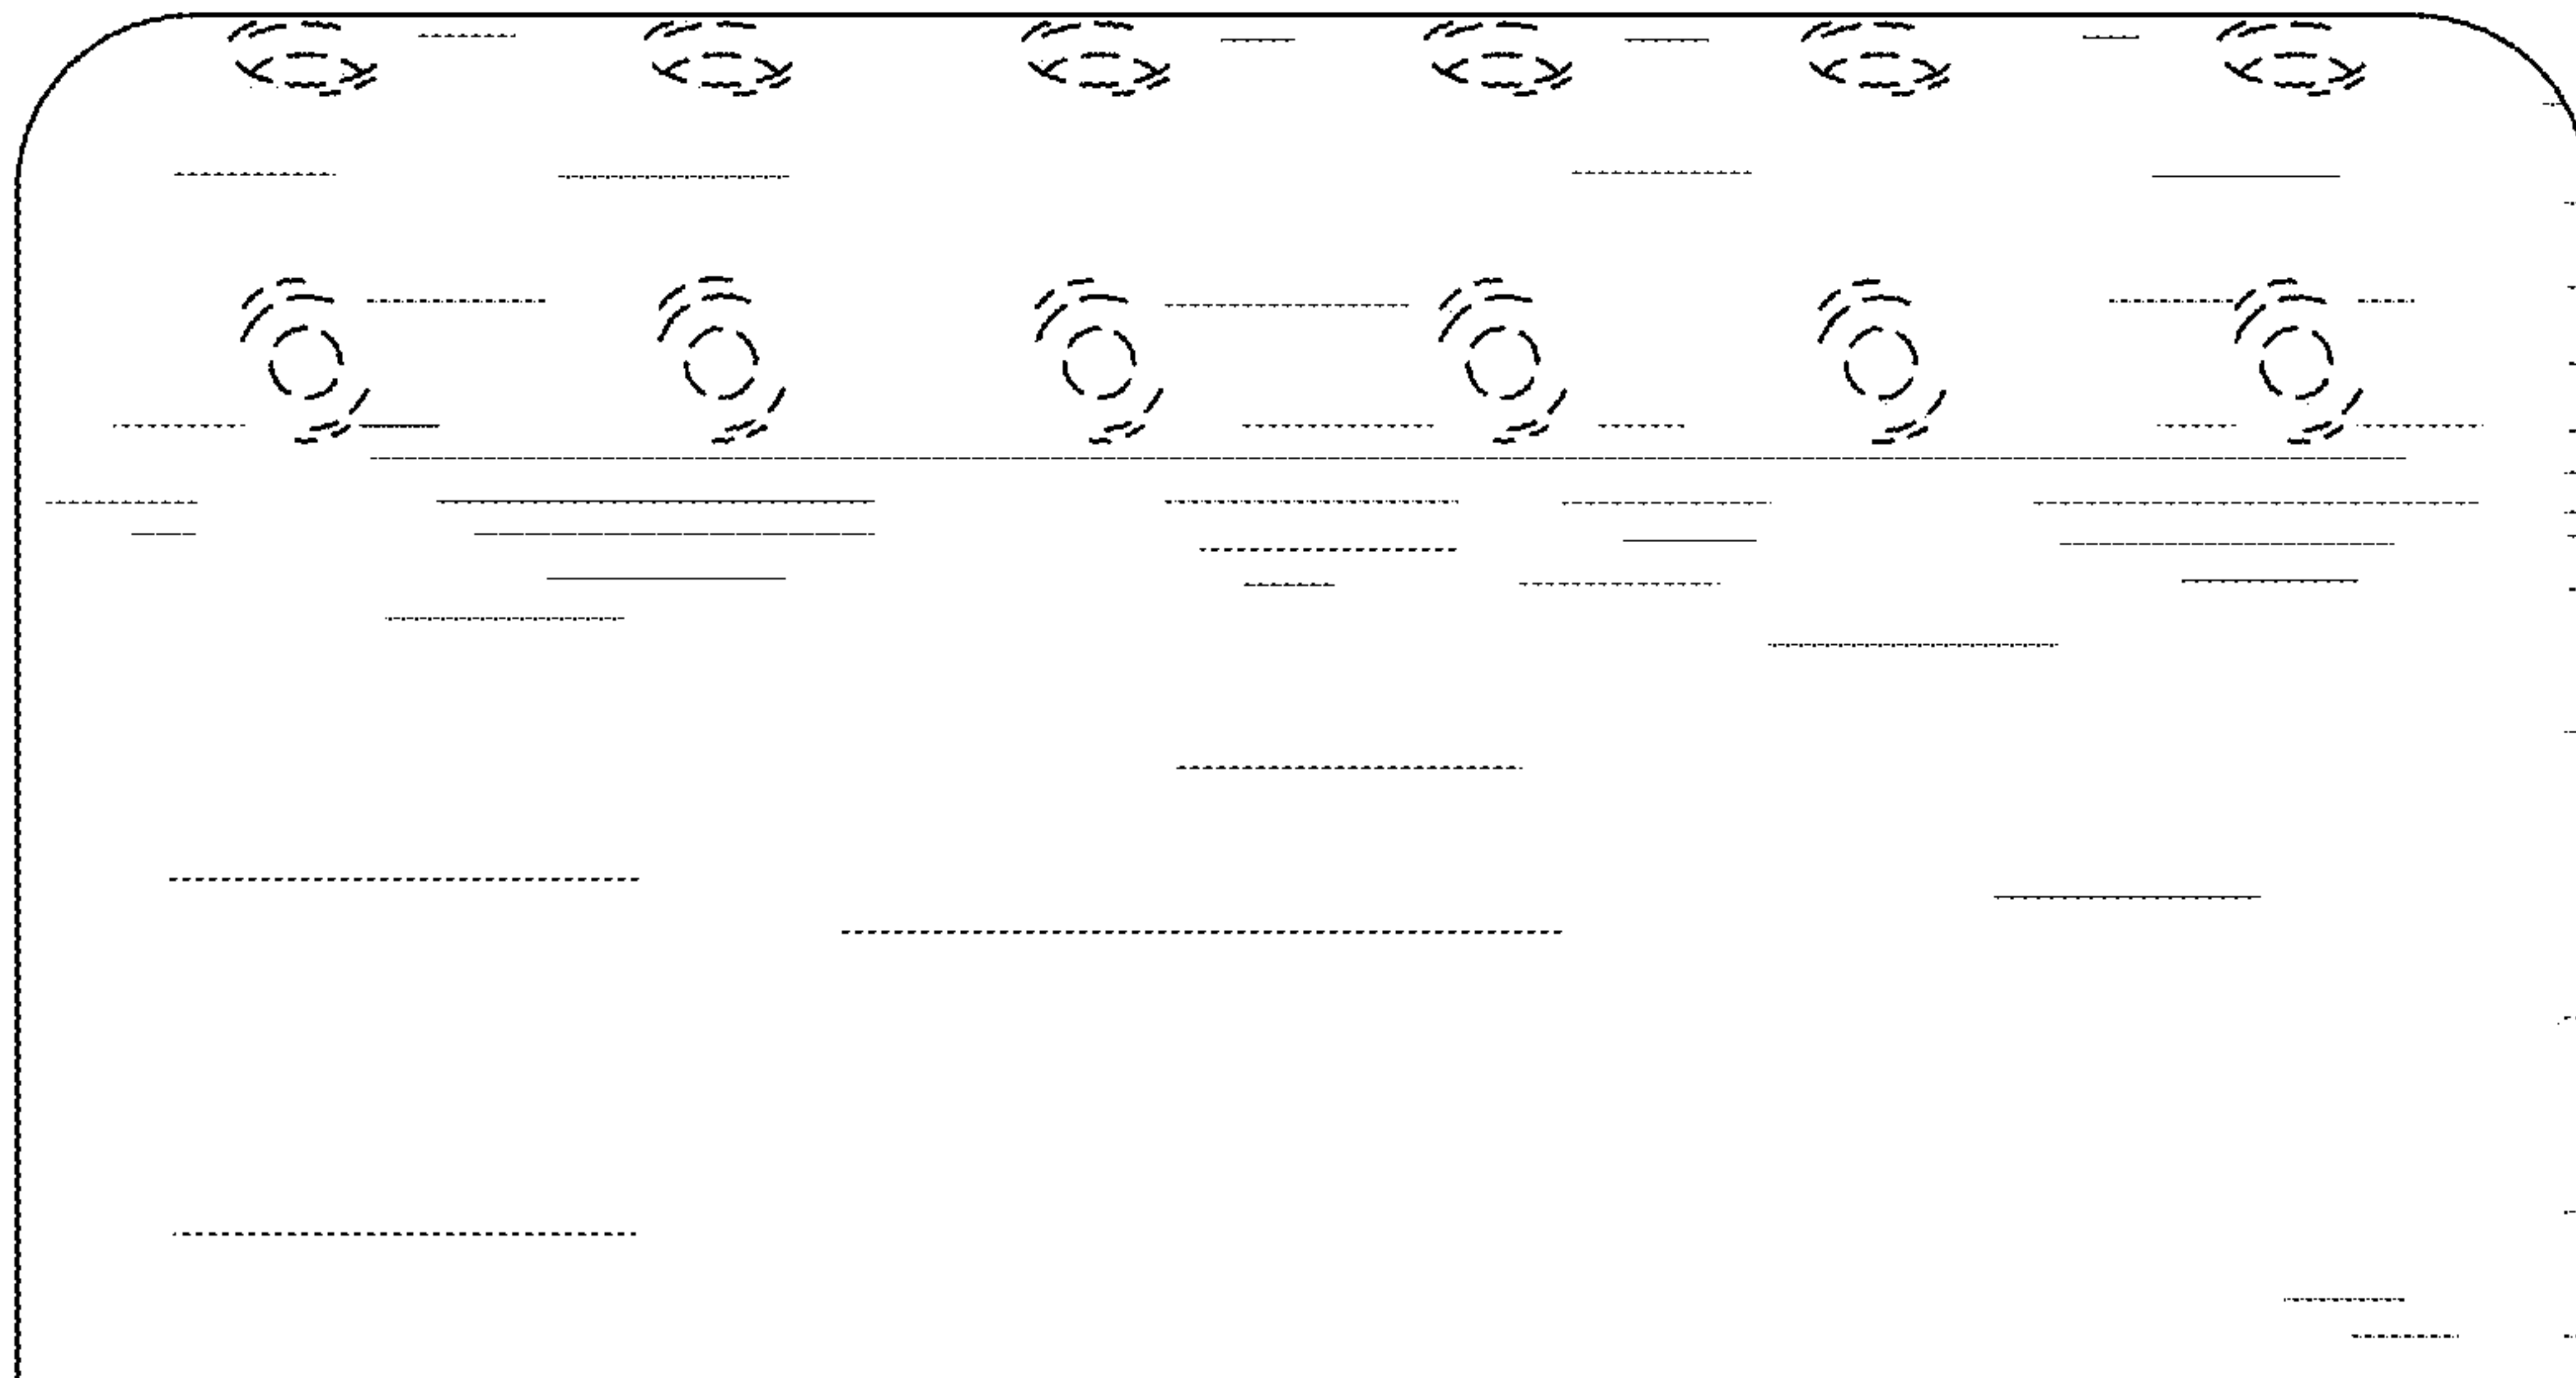


FIG. 3

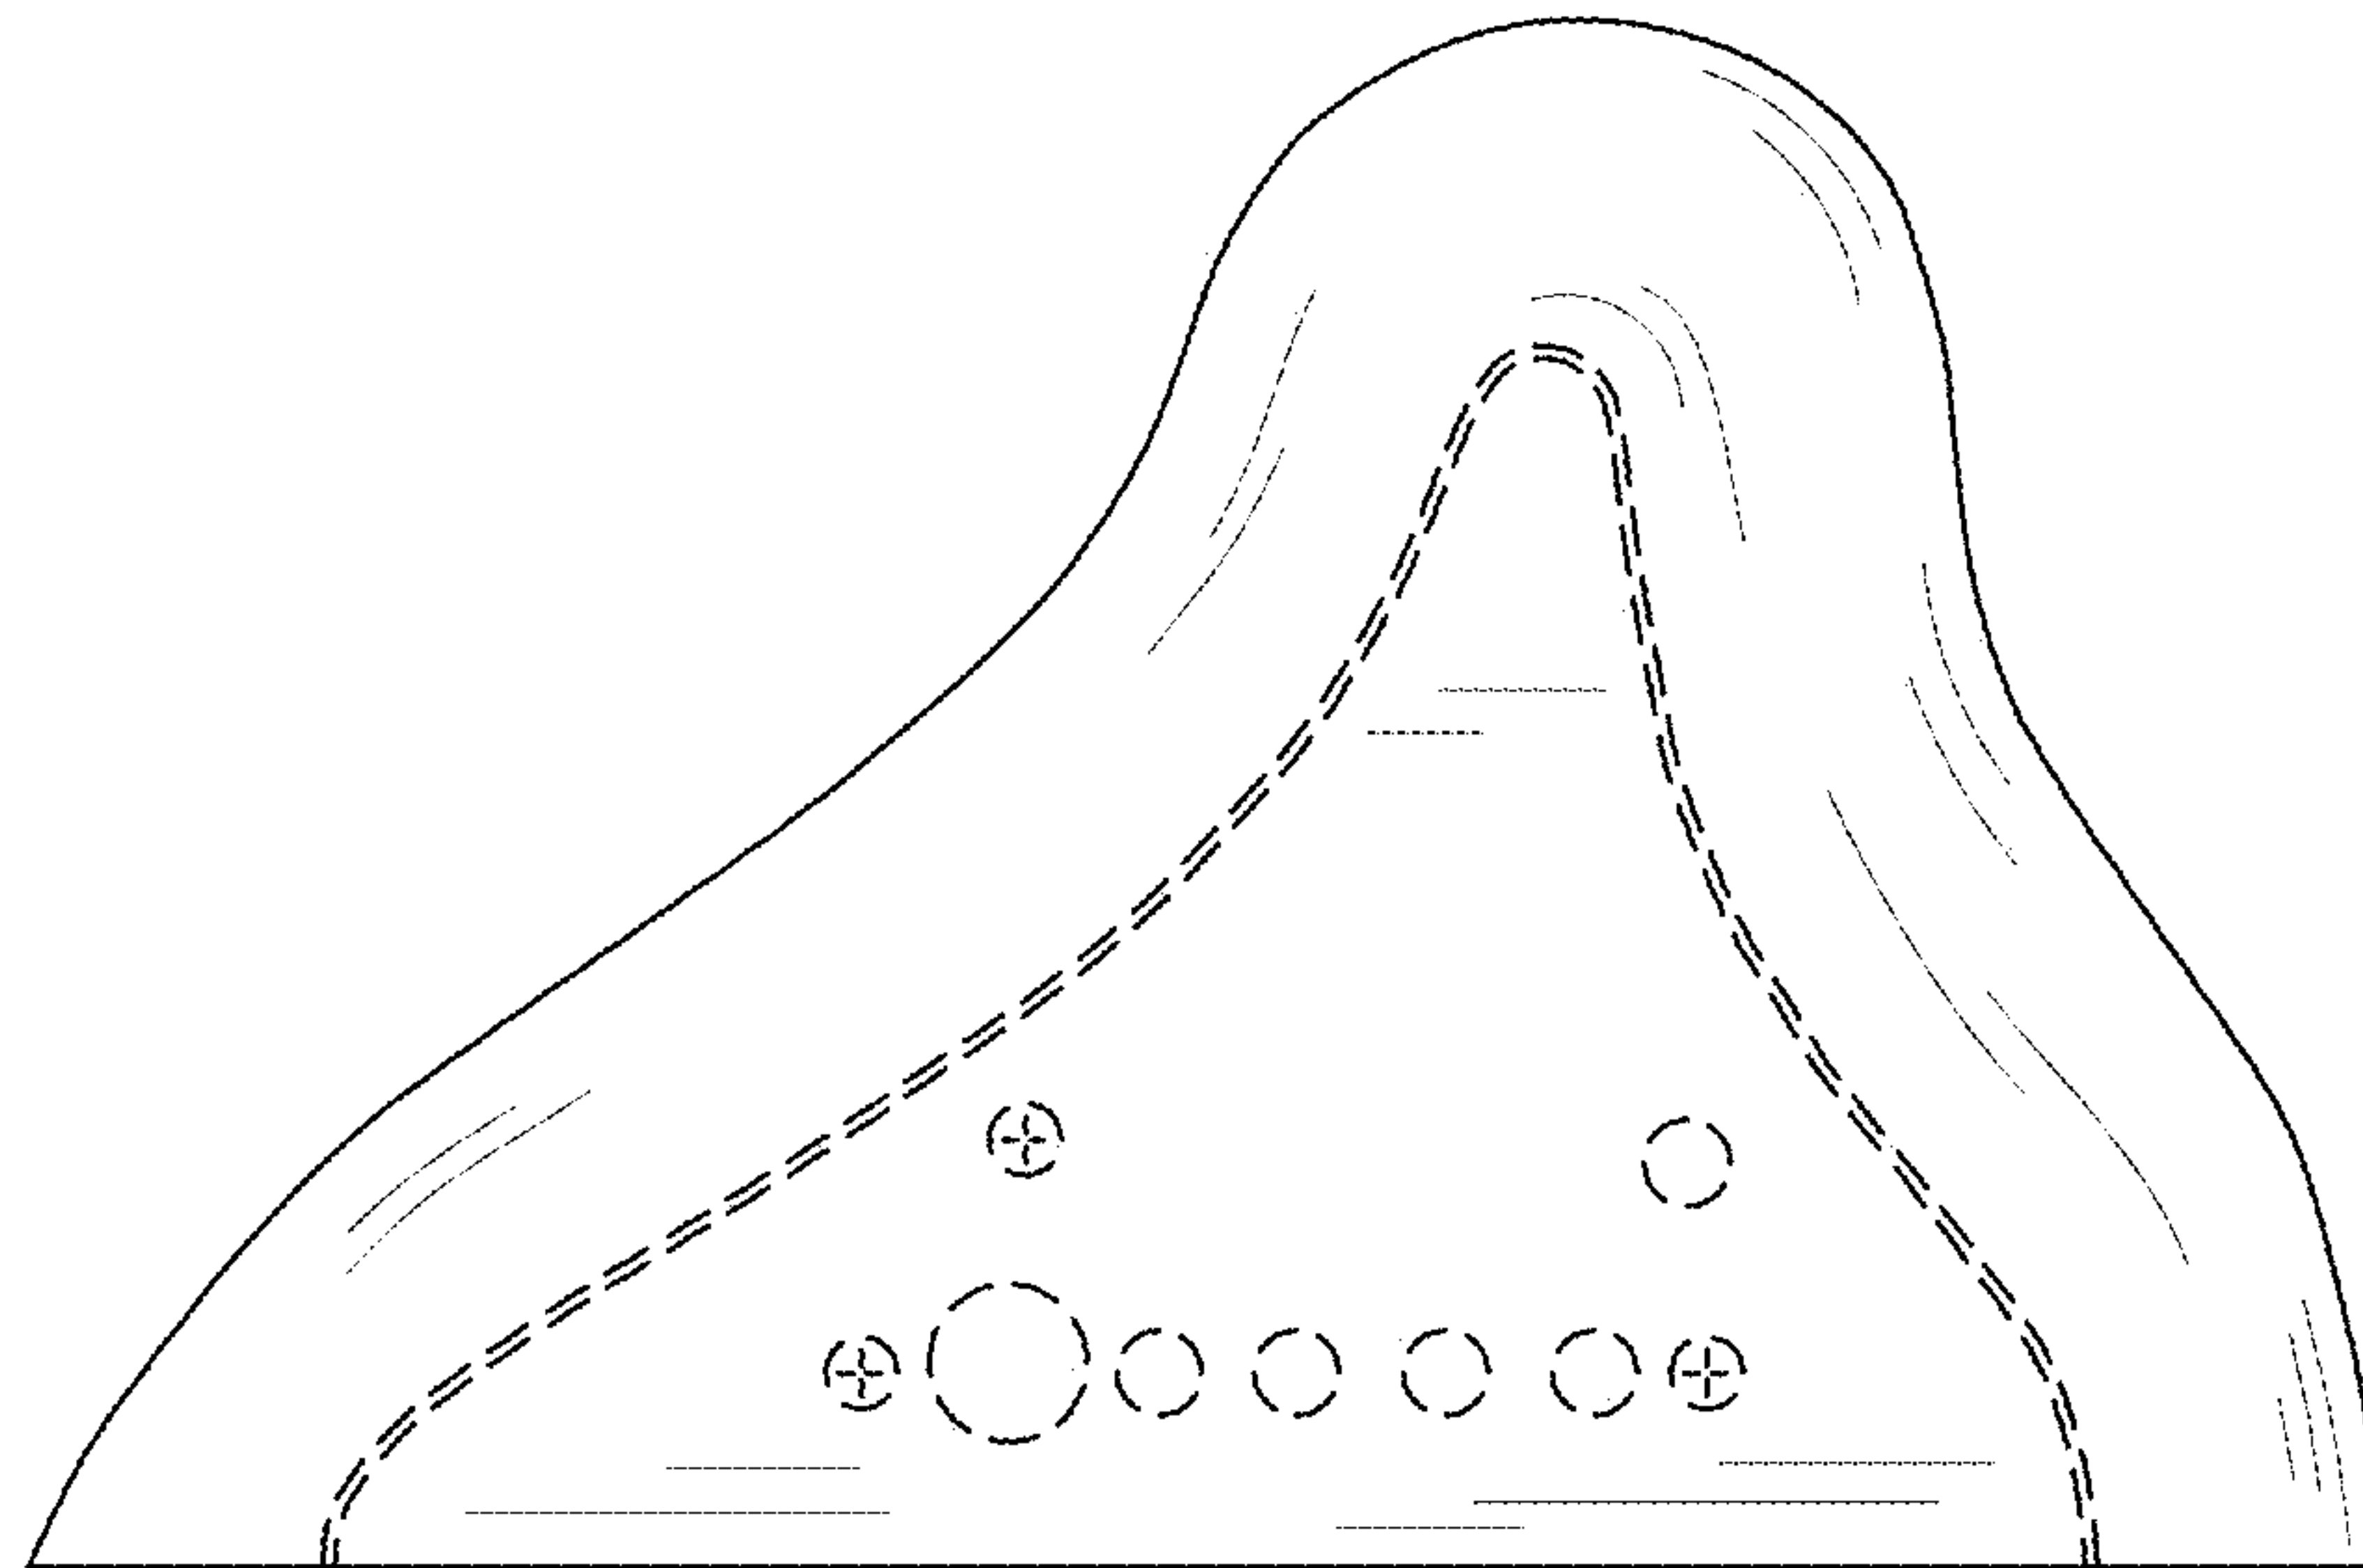


FIG. 4

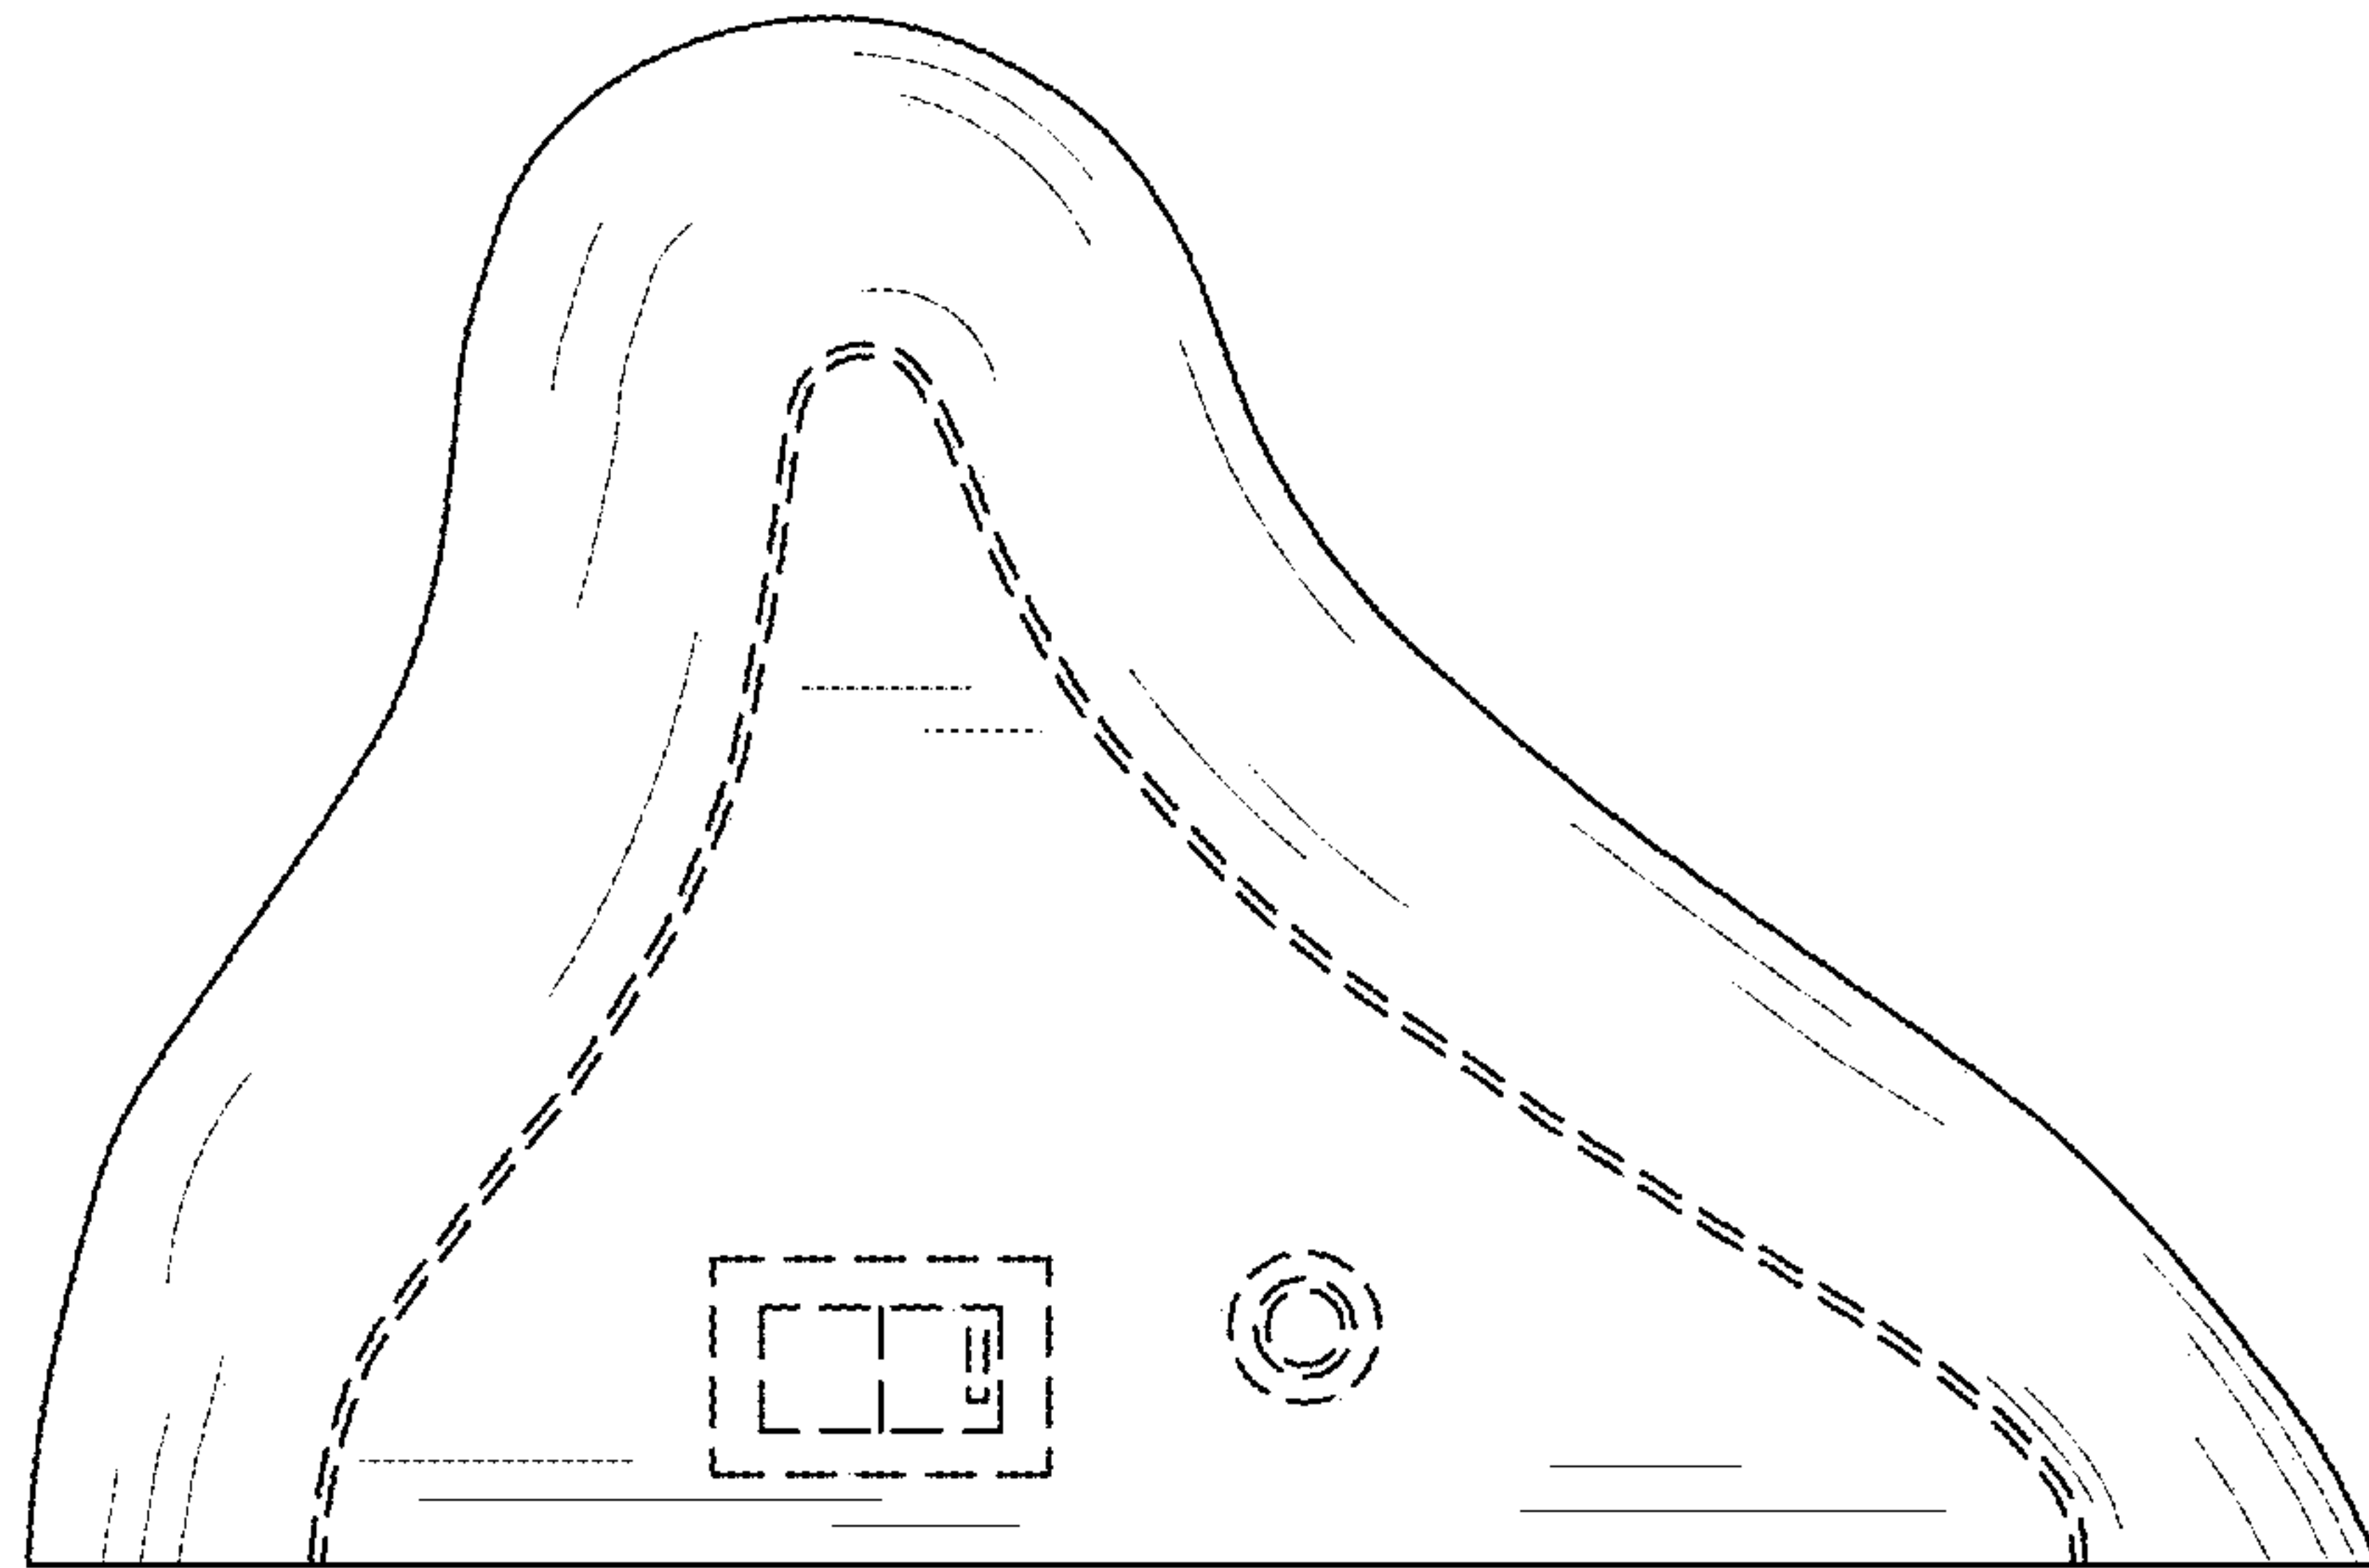


FIG. 5



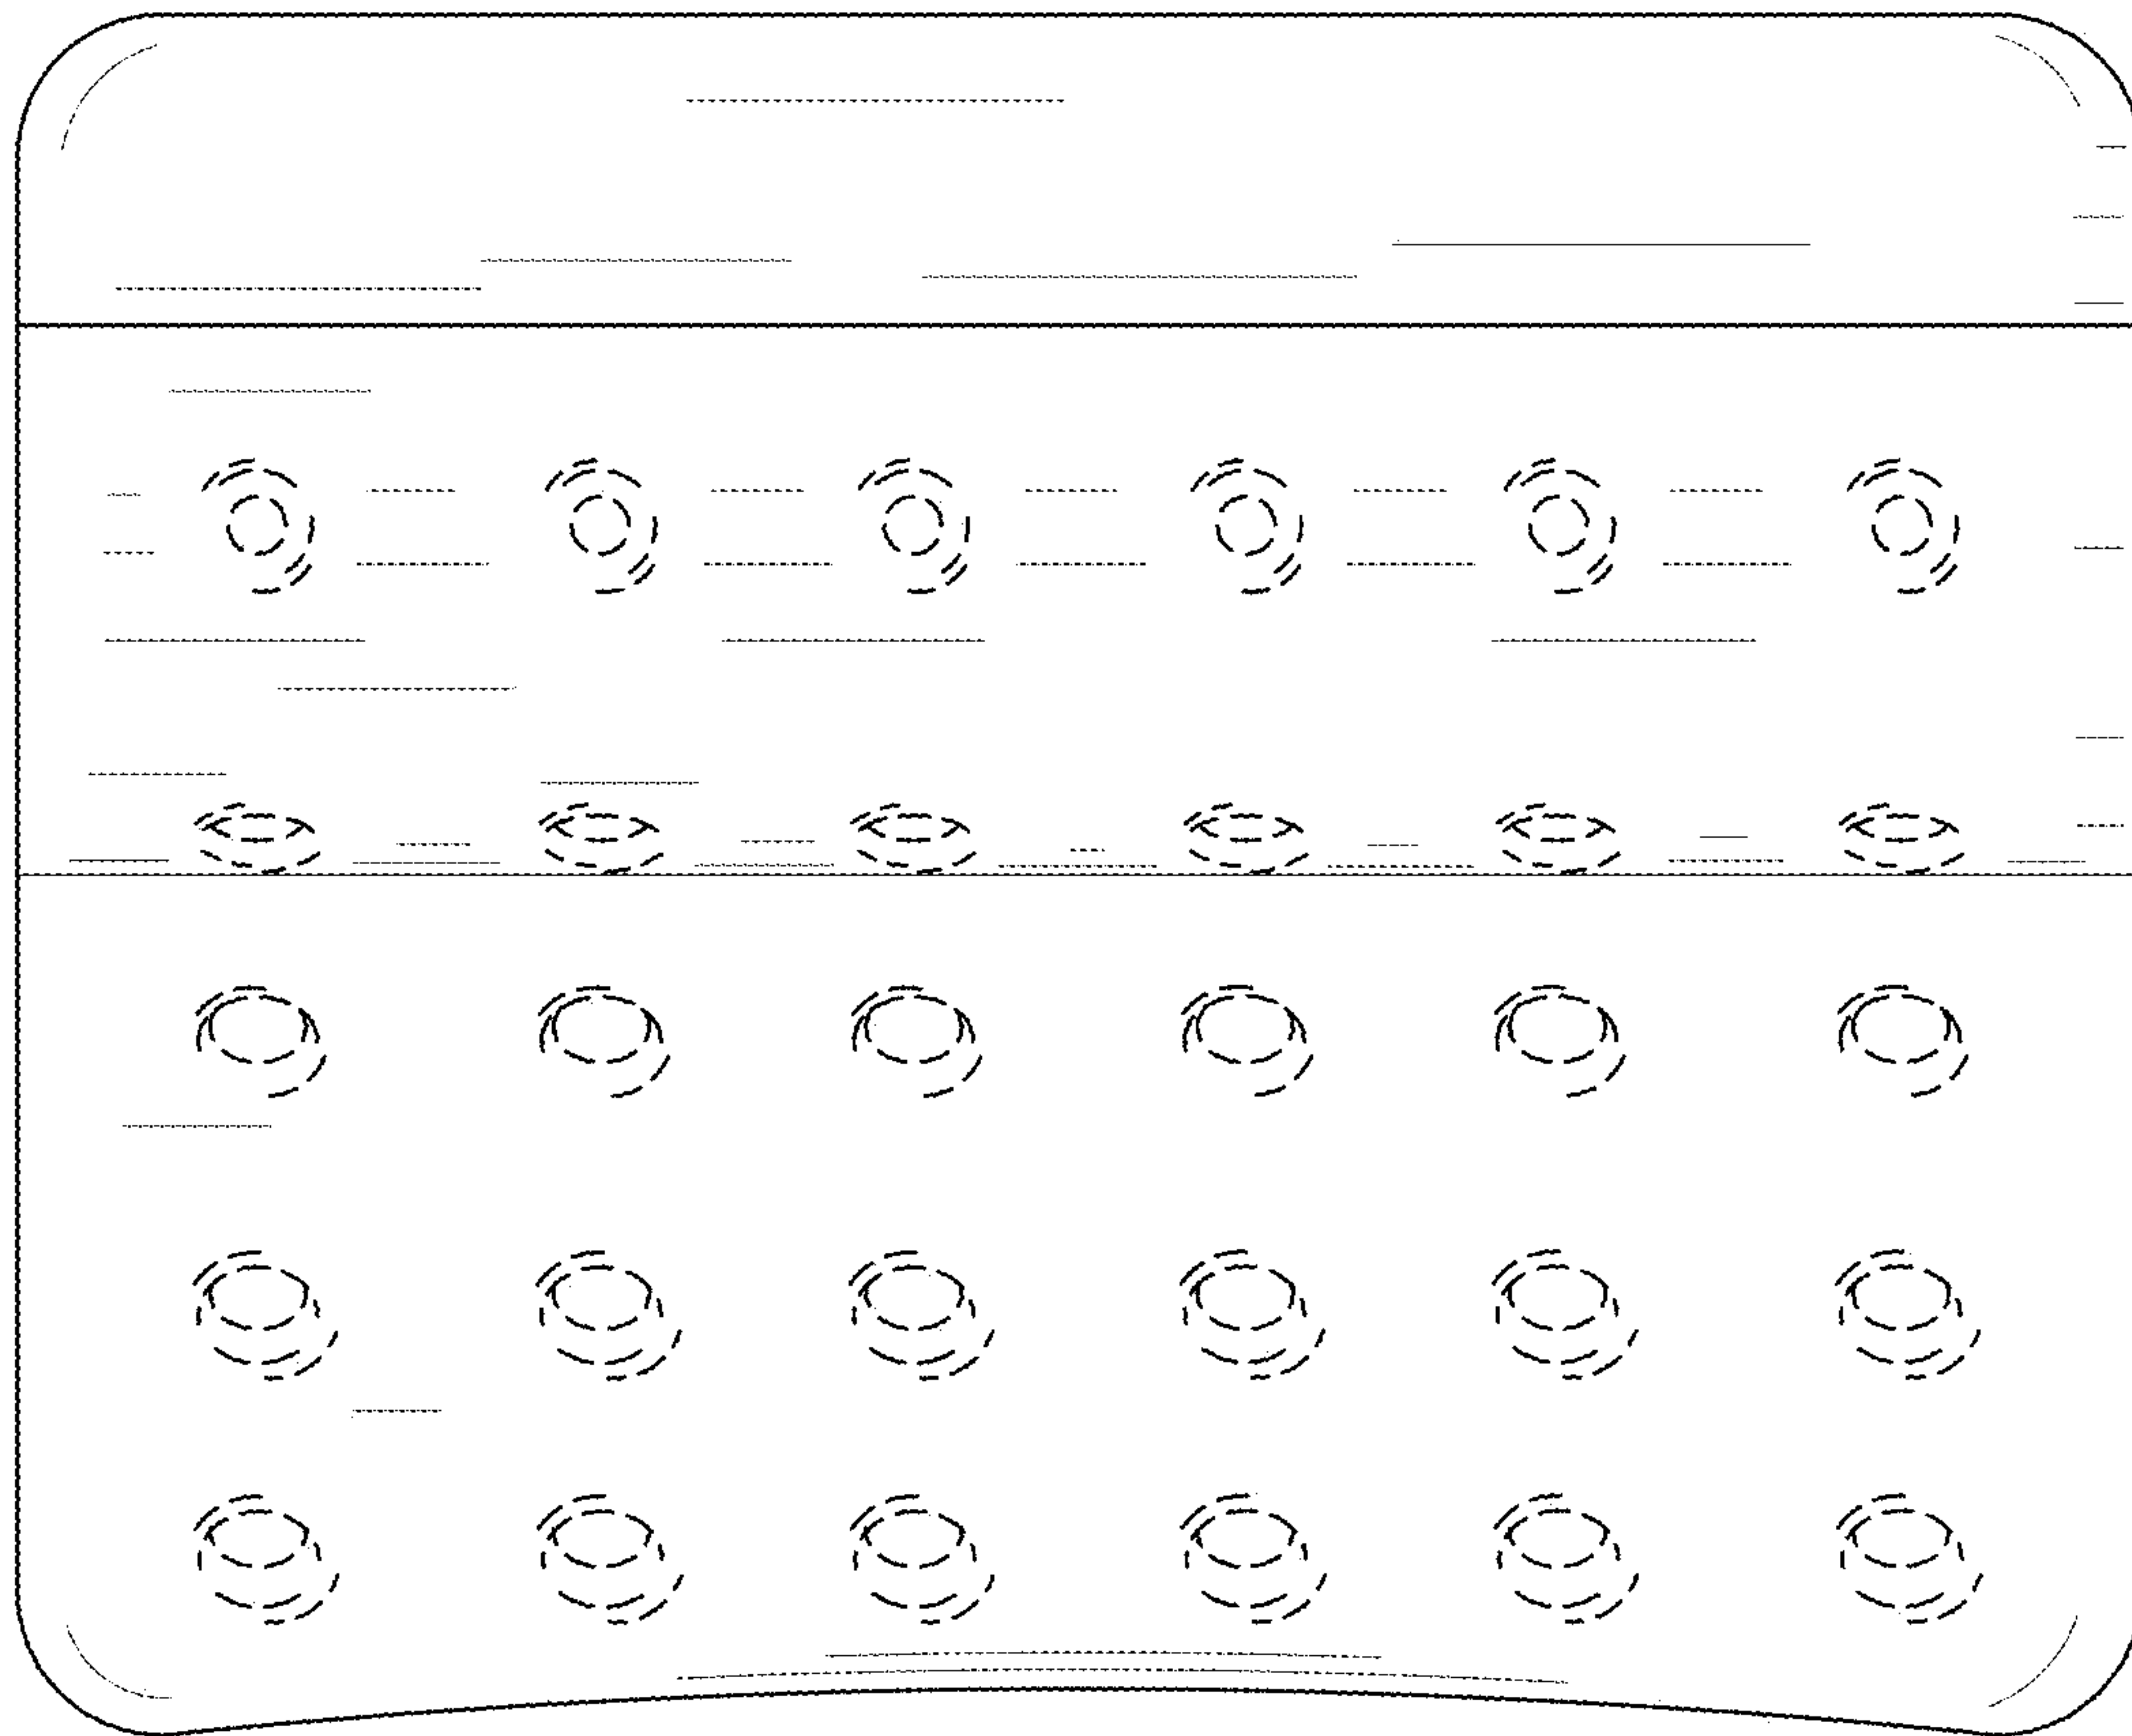


FIG. 6