



US0D1010832S

(12)

United States Design Patent

Masko et al.

(10)

Patent No.:

US D1,010,832 S

(45)

Date of Patent:

** Jan. 9, 2024

(54) MEDICAL ELECTRODE

(71) Applicant: i-Lumen Scientific, Inc., Bloomington, MN (US)

(72) Inventors: Marshall T. Masko, Minnetonka, MN (US); John C. Velure, Minnetonka, MN (US); Thu-Ha Duncan, Cleveland, TN (US)

(73) Assignee: i-Lumen Scientific, Inc., Bloomington, MN (US)

(**) Term: 15 Years

(21) Appl. No.: 29/817,501

(22) Filed: Dec. 1, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/187

(58) Field of Classification Search USPC D24/107, 168, 186, 187, 189, 200 CPC ... A61B 5/0404; A61B 5/0416; A61B 5/0422; A61B 5/0424; A61B 5/04012; A61B 5/04082; A61B 5/04085; A61B 5/04087; A61B 5/6841; A61N 1/046; A61N 1/0472; A61N 1/0476 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

6,298,255 B1 * 10/2001 Cordero A61B 5/303 600/372

8,188,433 B2 * 5/2012 Gonopolskiy A61B 5/68335 600/344

D779,432 S * 2/2017 Wong D13/133

D854,697	S	*	7/2019	Yang	D24/187
D860,465	S	*	9/2019	Lovell	D24/187
D880,701	S	*	4/2020	Oz	D14/344
D905,858	S	*	12/2020	Lovell	D24/187
D927,005	S	*	8/2021	Hauser-Raspe	D24/200
D936,843	S	*	11/2021	Besko	D24/187
D970,018	S	*	11/2022	Soosalu	D24/186
D971,415	S	*	11/2022	Treen	D24/187

OTHER PUBLICATIONS

I-Lumen Scientific, Inc—Virtual Rocket Pitch presentation at Connectpreneur. Online, published date Oct. 14, 2021. Retrieved on Jul. 21, 2023 from URL: https://www.youtube.com/watch?v=iv6vA7D_ngo.*

* cited by examiner

Primary Examiner — Omeed Agilee
(74) Attorney, Agent, or Firm — Jonathan M. Rixen; Charles A. Lemaire; Lemaire Patent Law Firm, P.L.L.C.

(57) CLAIM

The ornamental design for a medical electrode, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical electrode showing our new design;
FIG. 2 is a top view thereof;
FIG. 3 is a left-side view thereof;
FIG. 4 is a bottom view thereof;
FIG. 5 is a right-side view thereof;
FIG. 6 is a back view thereof; and,
FIG. 7 is a front view thereof.
In FIGS. 1-7, the broken lines are for the purpose of illustrating portions of the medical electrode that are not part of the claimed design.

1 Claim, 2 Drawing Sheets

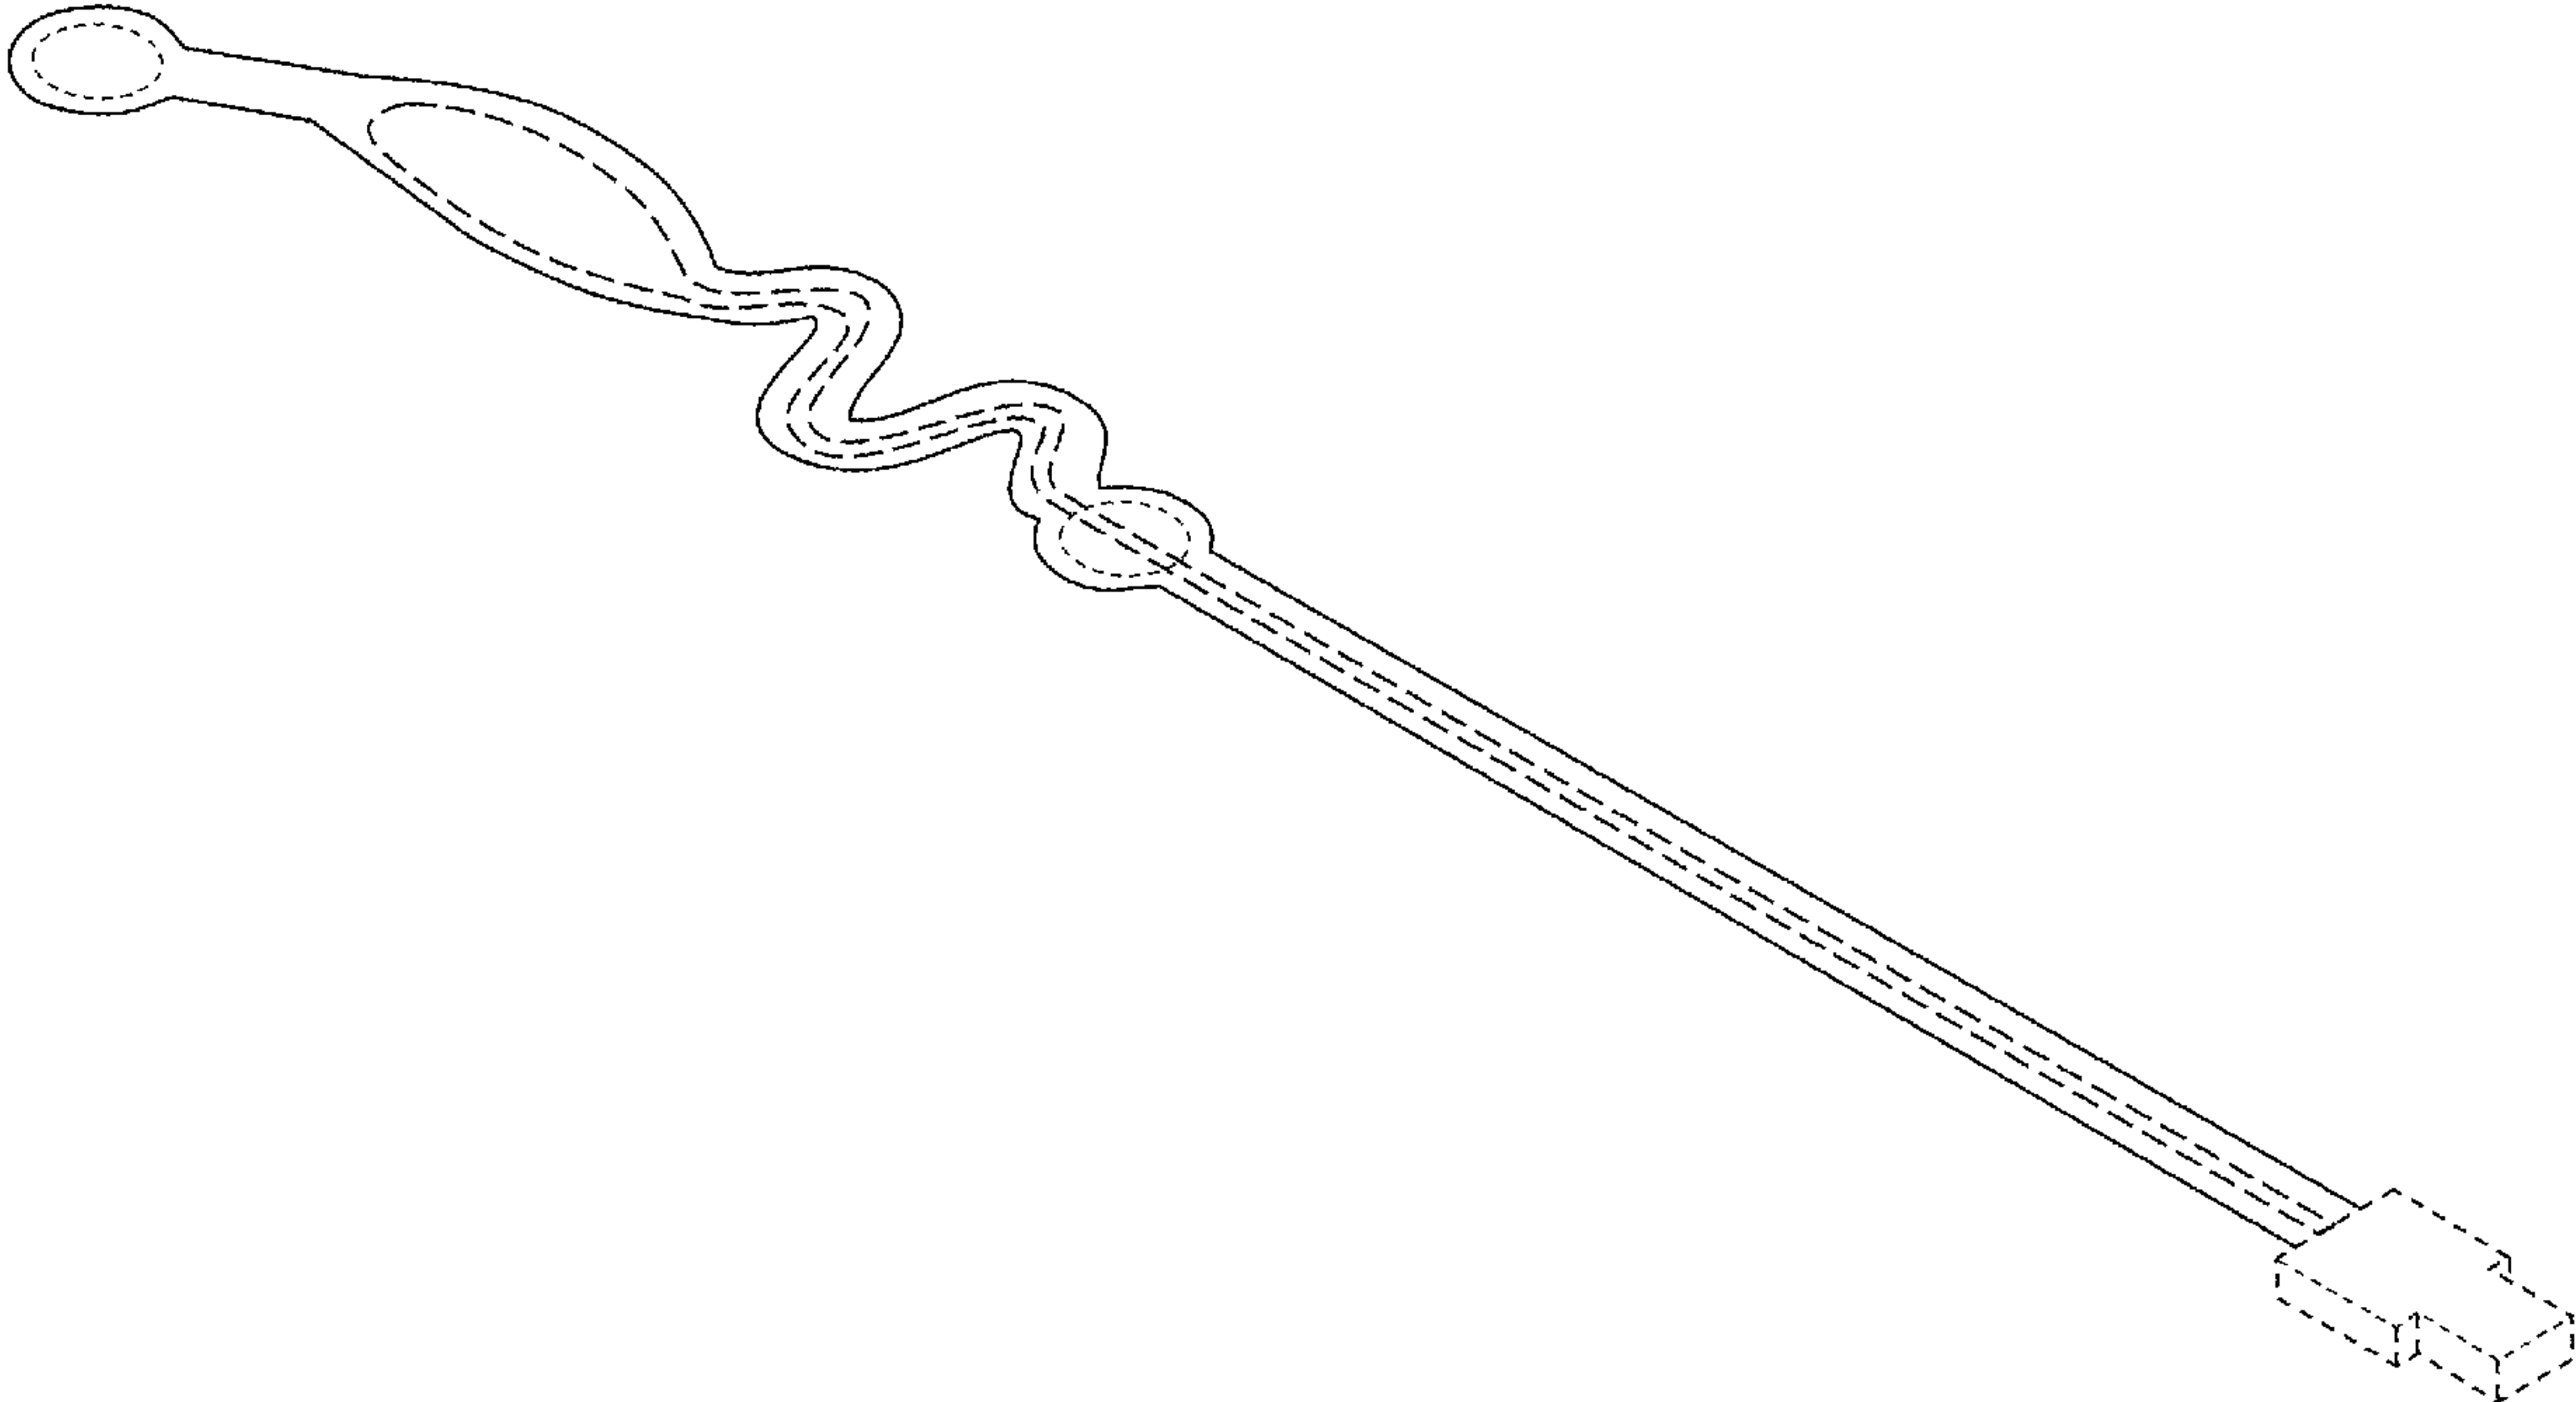


FIG. 1

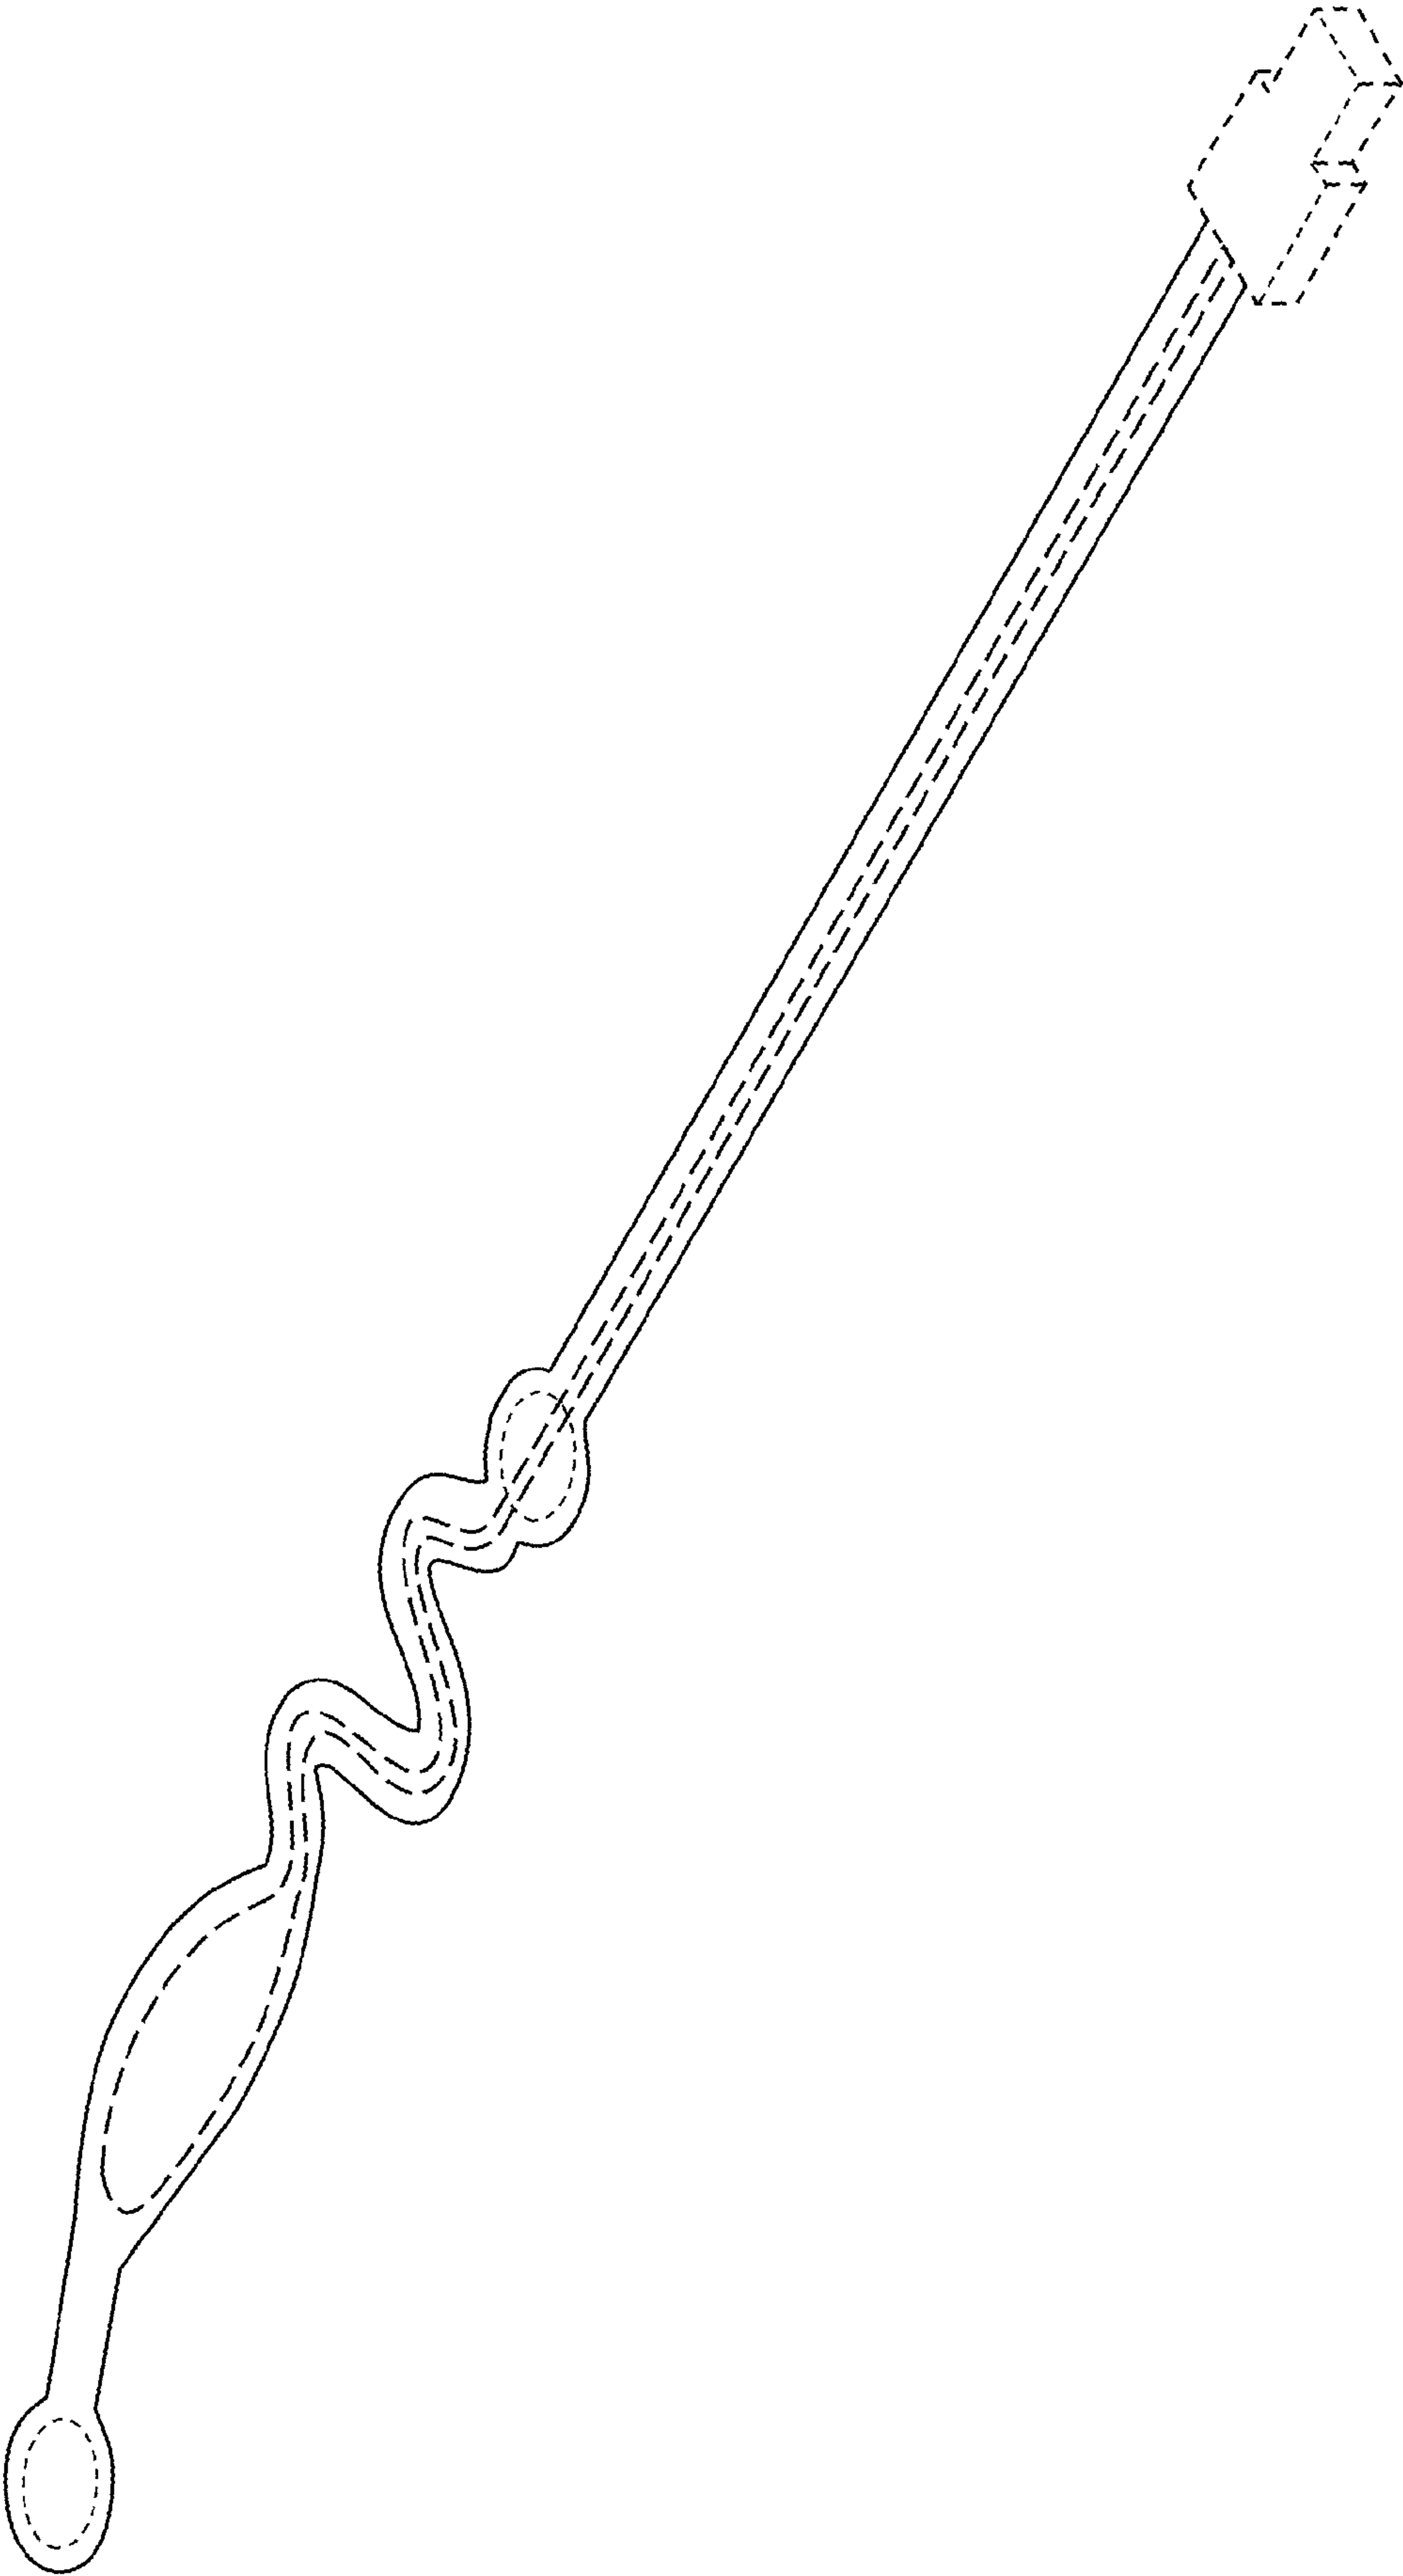


FIG. 6



FIG. 7

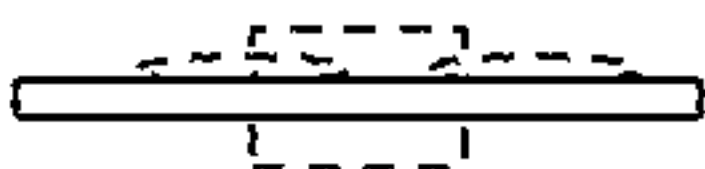


FIG. 2

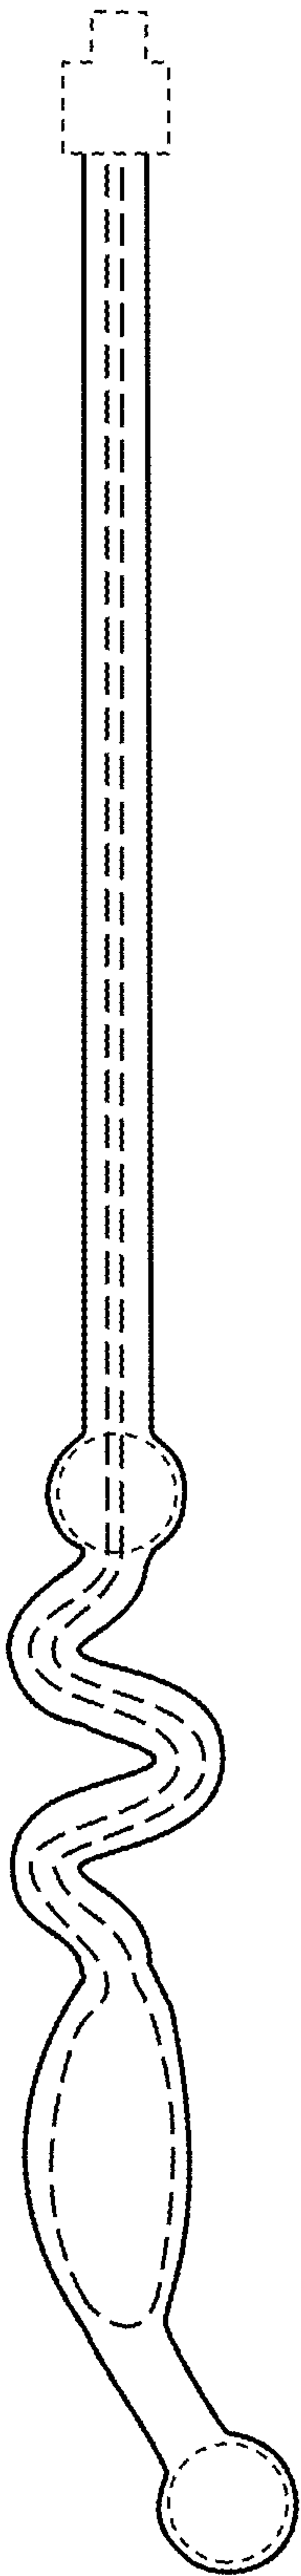


FIG. 3

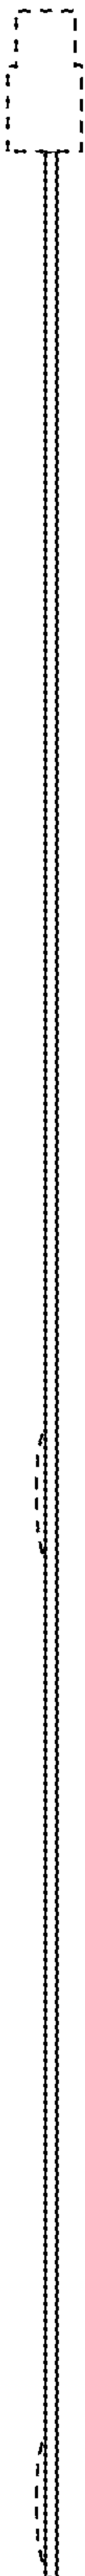


FIG. 4

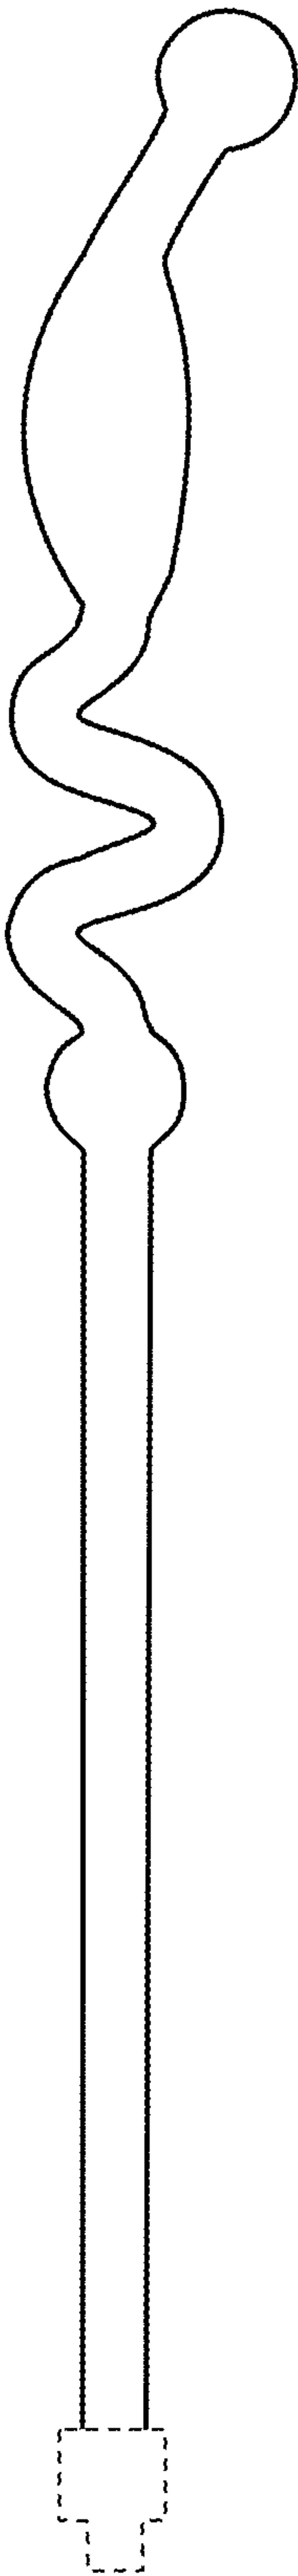


FIG. 5

