

US0D1011524S

(12)

United States Design Patent

Santrock et al.

(10)

Patent No.:

US D1,011,524 S

(45)

Date of Patent:

** Jan. 16, 2024

(54) COMPRESSOR-DISTRACTOR FOR THE FOOT

(71) Applicant: Treace Medical Concepts, Inc., Ponte Vedra, FL (US)

(72) Inventors: Robert D. Santrock, Morgantown, WV (US); Adriaan Kuyler, Ponte Vedra, FL (US); Jody McAleer, Jefferson City, MO (US); William DeCarbo, Pittsburgh, PA (US)

4,349,018 A 9/1982 Chambers

4,409,973 A 10/1983 Neufeld

4,440,168 A 4/1984 Warren

4,501,268 A 2/1985 Comparetto

(Continued)

FOREIGN PATENT DOCUMENTS

AU 2009227957 B2 7/2014

CA 2491824 A1 9/2005

(Continued)

OTHER PUBLICATIONS

Sidekick Stealth Rearfoot Fixator, Wright Medical Technology, Surgical Technique, Dec. 2, 2013, 20 pages.

(Continued)

(**) Term: 15 Years

(21) Appl. No.: 29/827,986

(22) Filed: Feb. 23, 2022

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/135

(58) Field of Classification Search USPC D24/135, 133, 112, 113, 129, 137, 138, D24/140, 143 CPC . A61B 17/8866; A61B 17/17; A61B 17/1775; A61B 2017/681 See application file for complete search history.

Primary Examiner — Bridget L Eland

(74) Attorney, Agent, or Firm — Fredrikson & Byron, P.A.

(57) CLAIM

We claim the ornamental design for a compressor-distractor for the foot, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a compressor-distractor for the foot showing my new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof;

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

The dot-dash broken lines and evenly dashed broken lines adjacent the claim define the bounds of the claimed design and form no part thereof. The remainder of the evenly dashed broken lines shown on FIGS. 1-7 illustrate portions of the compressor-distractor for the foot that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

(56) References Cited

U.S. PATENT DOCUMENTS

2,251,209 A 7/1941 Stader

2,432,695 A 12/1947 Speas

3,664,022 A 5/1972 Small

4,069,824 A 1/1978 Weinstock


4,159,716 A 7/1979 Borchers

4,187,840 A 2/1980 Watanabe

4,187,841 A 2/1980 Knutson

4,335,715 A 6/1982 Kirkley

4,338,927 A 7/1982 Volkov et al.

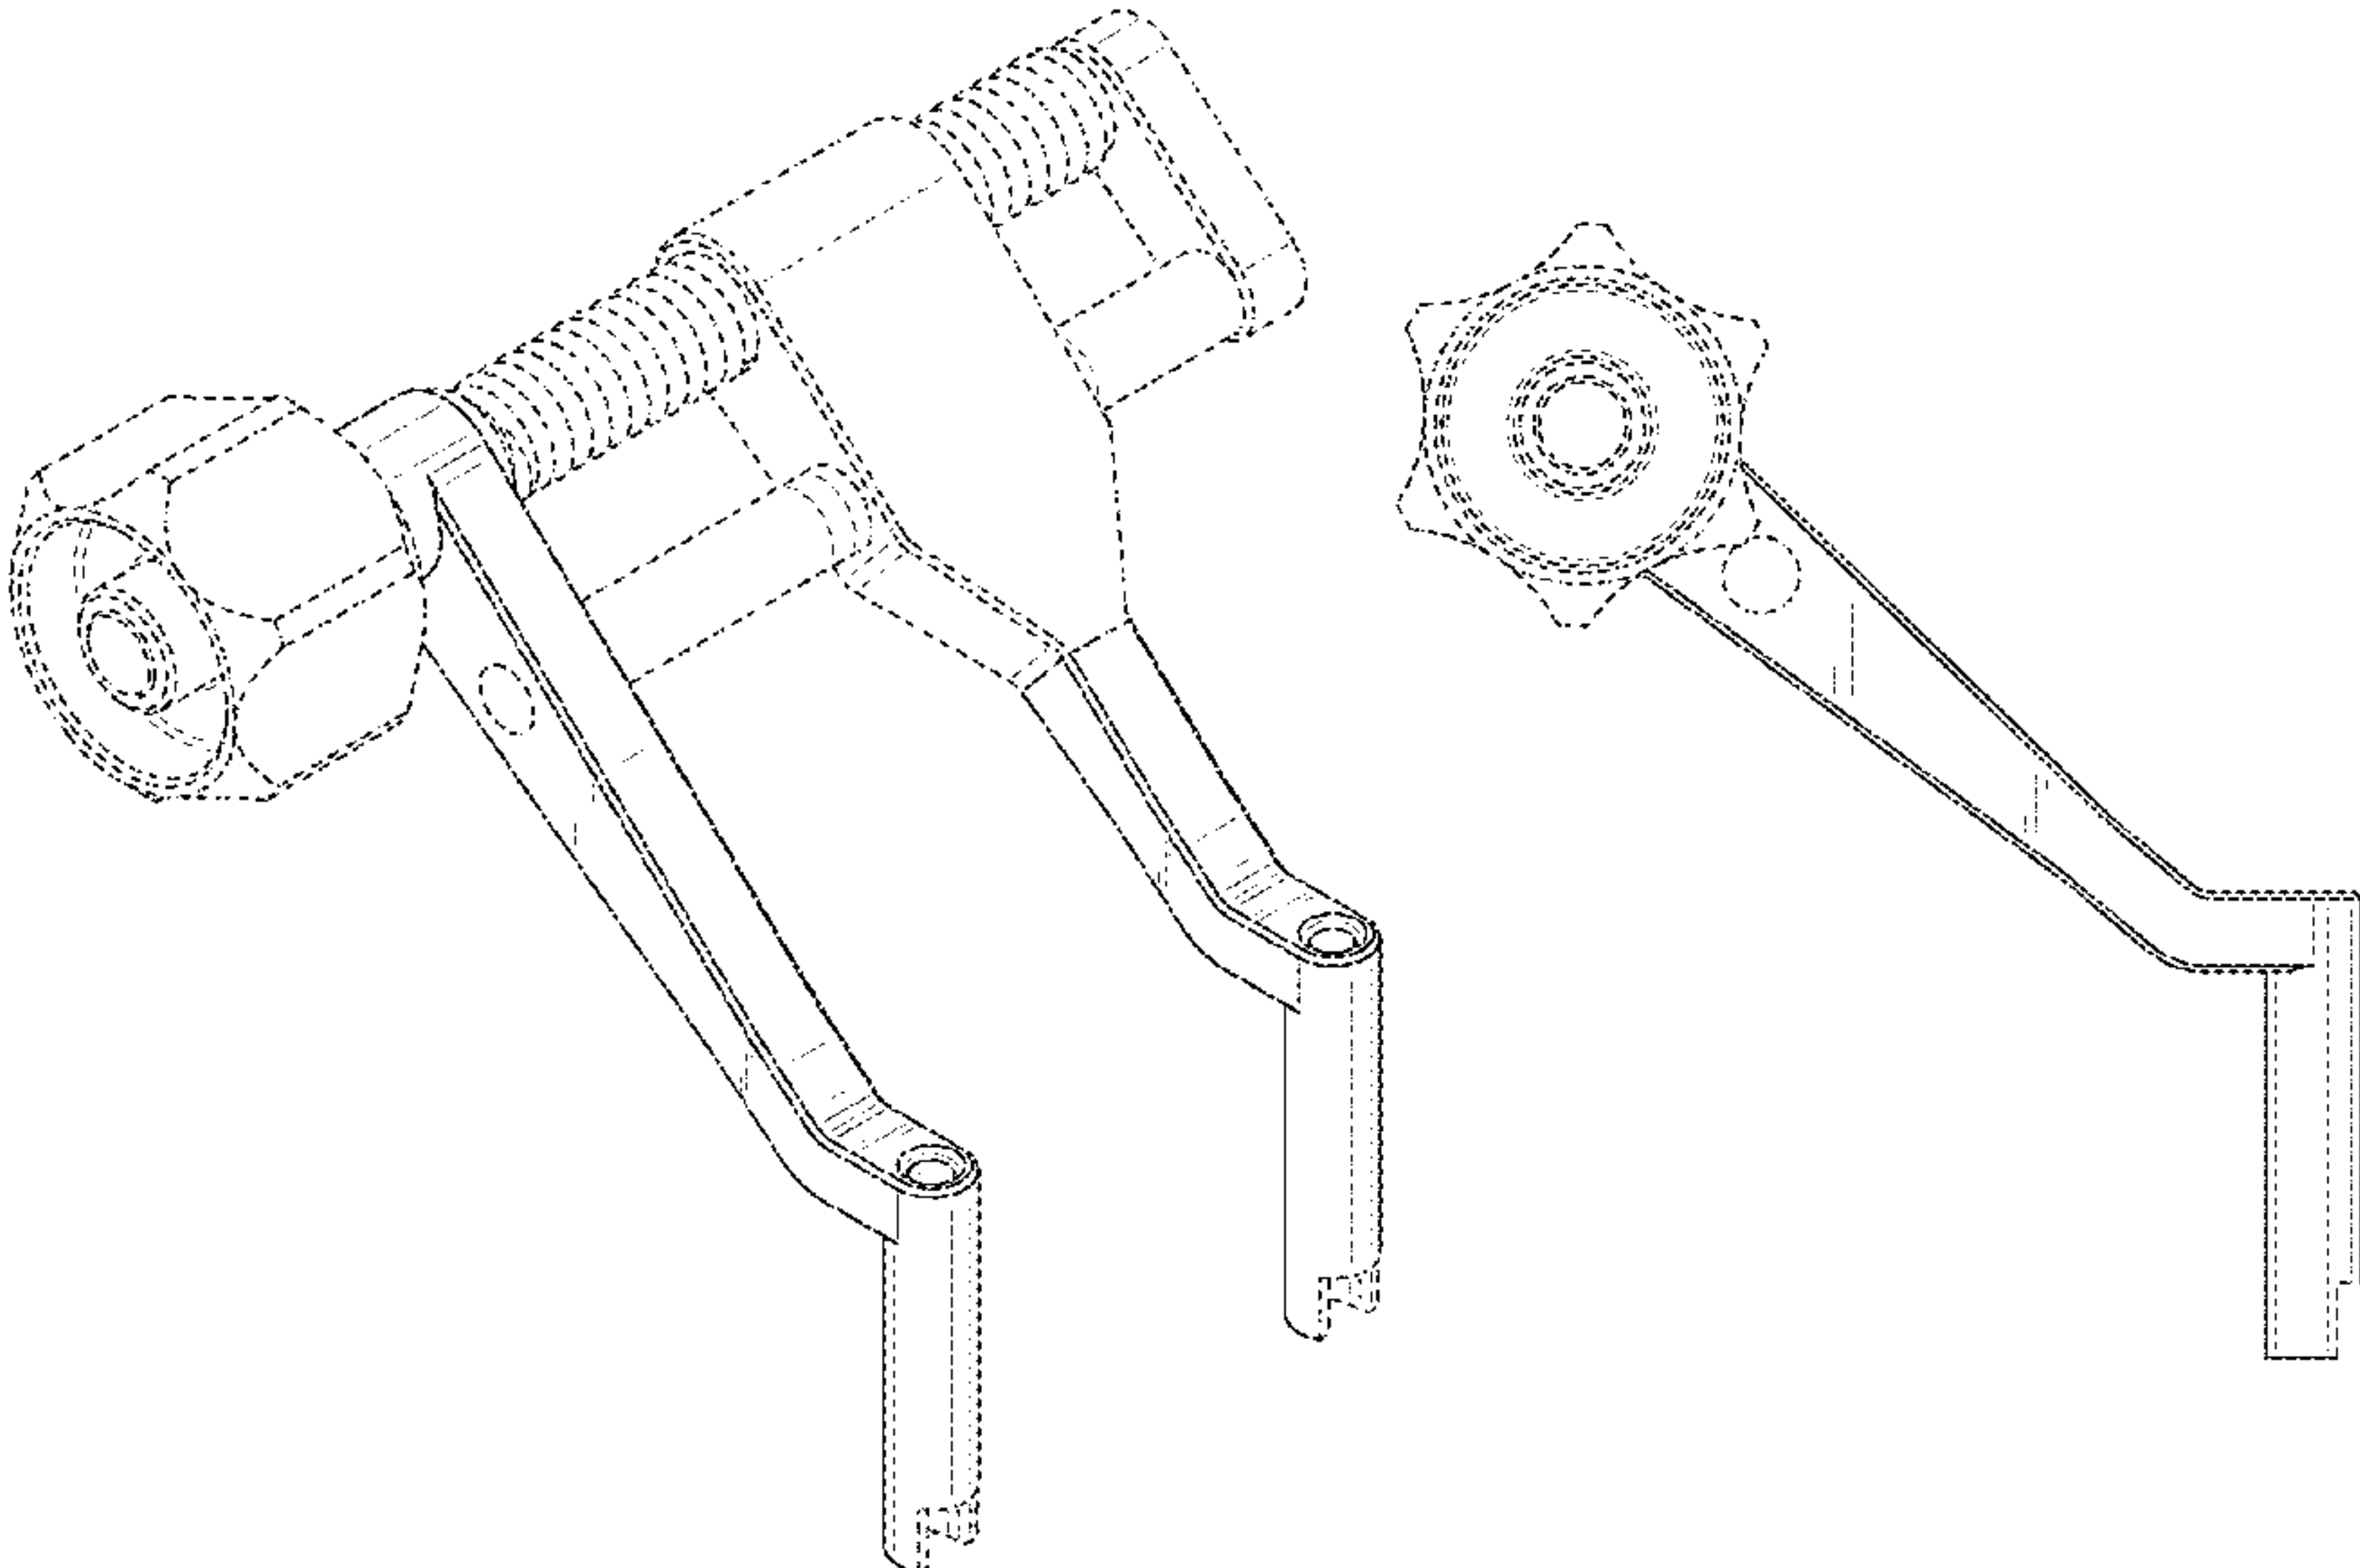

(56)

References Cited

U.S. PATENT DOCUMENTS

4,502,474 A	3/1985	Comparetto	6,416,465 B2	7/2002	Brau
4,509,511 A	4/1985	Neufeld	6,478,799 B1	11/2002	Williamson
4,565,191 A	1/1986	Slocum	6,511,481 B2	1/2003	Von Hoffmann et al.
4,570,624 A	2/1986	Wu	6,547,793 B1	4/2003	Mcguire
4,627,425 A	12/1986	Reese	6,676,662 B1	1/2004	Bagga et al.
4,628,919 A	12/1986	Clyburn	6,719,773 B1	4/2004	Boucher et al.
4,632,102 A	12/1986	Comparetto	6,743,233 B1	6/2004	Baldwin et al.
4,664,102 A	5/1987	Comparetto	6,755,838 B2	6/2004	Trnka
4,708,133 A	11/1987	Comparetto	6,796,986 B2	9/2004	Duffner
4,736,737 A	4/1988	Fargie et al.	6,859,661 B2	2/2005	Tuke
4,750,481 A	6/1988	Reese	7,018,383 B2	3/2006	Mcguire
4,754,746 A	7/1988	Cox	7,033,361 B2	4/2006	Collazo
4,757,810 A	7/1988	Reese	7,097,647 B2	8/2006	Segler
4,895,141 A	1/1990	Koeneman et al.	7,112,204 B2	9/2006	Justin et al.
4,952,214 A	8/1990	Comparetto	7,153,310 B2	12/2006	Ralph et al.
4,959,066 A	9/1990	Dunn et al.	7,182,766 B1	2/2007	Mogul
4,978,347 A	12/1990	Ilizarov	7,241,298 B2	7/2007	Nemec et al.
4,988,349 A	1/1991	Pennig	7,282,054 B2	10/2007	Steffensmeier et al.
4,995,875 A	2/1991	Coes	D566,271 S *	4/2008	Gao D24/143
5,021,056 A	6/1991	Hofmann et al.	7,377,924 B2	5/2008	Raistrick et al.
5,035,698 A	7/1991	Comparetto	7,465,303 B2	12/2008	Riccione et al.
5,042,983 A	8/1991	Rayhack	7,540,874 B2	6/2009	Trumble et al.
5,049,149 A	9/1991	Schmidt	7,572,258 B2	8/2009	Stiernborg
5,053,039 A	10/1991	Hofmann et al.	7,578,822 B2	8/2009	Rezach et al.
5,078,719 A	1/1992	Schreiber	7,618,424 B2	11/2009	Wilcox et al.
5,112,334 A	5/1992	Alchermes et al.	7,641,660 B2	1/2010	Lakin et al.
5,147,364 A	9/1992	Comparetto	D610,257 S	2/2010	Horton
5,176,685 A	1/1993	Rayhack	7,686,811 B2	3/2010	Byrd et al.
5,207,676 A	5/1993	Canadell et al.	7,691,108 B2	4/2010	Lavallee
5,246,444 A	9/1993	Schreiber	7,763,026 B2	7/2010	Egger et al.
5,254,119 A	10/1993	Schreiber	D629,900 S	12/2010	Fisher
5,304,177 A	4/1994	Pennig	7,967,823 B2	6/2011	Ammann et al.
5,312,412 A	5/1994	Whipple	7,972,338 B2	7/2011	O'Brien
5,358,504 A	10/1994	Paley et al.	D646,389 S	10/2011	Claypool et al.
5,364,402 A	11/1994	Mumme et al.	8,057,478 B2	11/2011	Kuczynski et al.
5,374,271 A	12/1994	Hwang	8,062,301 B2	11/2011	Ammann et al.
5,413,579 A	5/1995	Du Toit	D651,315 S	12/2011	Bertoni et al.
5,417,694 A	5/1995	Marik et al.	D651,316 S	12/2011	May et al.
5,449,360 A	9/1995	Schreiber	8,080,010 B2	12/2011	Schulz et al.
5,470,335 A	11/1995	Du Toit	8,080,045 B2	12/2011	Wotton, III
5,490,854 A	2/1996	Fisher et al.	8,083,746 B2	12/2011	Novak
5,529,075 A	6/1996	Clark	8,123,753 B2	2/2012	Poncet
5,540,695 A	7/1996	Levy	8,137,406 B2	3/2012	Novak et al.
5,578,038 A	11/1996	Barclay	8,147,530 B2	4/2012	Strnad et al.
5,586,564 A	12/1996	Barrett et al.	8,167,918 B2	5/2012	Strnad et al.
5,601,565 A	2/1997	Huebner	8,172,848 B2	5/2012	Tomko et al.
5,613,969 A	3/1997	Jenkins, Jr.	8,192,441 B2	6/2012	Collazo
5,620,442 A	4/1997	Bailey et al.	8,197,487 B2	6/2012	Poncet et al.
5,620,448 A	4/1997	Puddu	8,231,623 B1	7/2012	Jordan
D380,548 S *	7/1997	Koros D24/135	8,231,663 B2	7/2012	Kay et al.
5,643,270 A	7/1997	Combs	8,236,000 B2	8/2012	Ammann et al.
5,667,510 A	9/1997	Combs	8,246,561 B1	8/2012	Agee et al.
H1706 H	1/1998	Mason	D666,721 S	9/2012	Wright et al.
5,722,978 A	3/1998	Jenkins, Jr.	8,262,664 B2	9/2012	Justin et al.
5,749,875 A	5/1998	Puddu	8,277,459 B2	10/2012	Sand et al.
5,779,709 A	7/1998	Harris, Jr. et al.	8,282,644 B2	10/2012	Edwards
5,788,695 A	8/1998	Richardson	8,282,645 B2	10/2012	Lawrence et al.
5,803,924 A	9/1998	Akindele et al.	8,292,966 B2	10/2012	Morton
5,810,822 A	9/1998	Mortier	8,303,596 B2	11/2012	Plaky et al.
5,843,085 A	12/1998	Graser	8,313,492 B2	11/2012	Wong et al.
5,893,553 A	4/1999	Pinkous	8,323,289 B2	12/2012	Re
5,911,724 A	6/1999	Wehrli	8,337,503 B2	12/2012	Lian
5,935,128 A	8/1999	Carter et al.	8,343,159 B2	1/2013	Bennett
5,941,877 A	8/1999	Viegas et al.	8,377,105 B2	2/2013	Bscher
5,951,556 A	9/1999	Faccioli et al.	D679,395 S	4/2013	Wright et al.
5,980,526 A	11/1999	Johnson et al.	8,409,209 B2	4/2013	Ammann et al.
5,984,931 A	11/1999	Greenfield	8,435,246 B2	5/2013	Fisher et al.
6,007,535 A	12/1999	Rayhack et al.	8,475,462 B2	7/2013	Thomas et al.
6,027,504 A	2/2000	Mcguire	8,496,662 B2	7/2013	Novak et al.
6,030,391 A	2/2000	Brainard et al.	8,518,045 B2	8/2013	Szanto
6,162,223 A	12/2000	Orsak et al.	8,523,870 B2	9/2013	Green, II et al.
6,171,309 B1	1/2001	Huebner	8,529,571 B2	9/2013	Horan et al.
6,203,545 B1	3/2001	Stoffella	8,540,777 B2	9/2013	Ammann et al.
6,248,109 B1	6/2001	Stoffella	8,545,508 B2	10/2013	Collazo
6,391,031 B1	5/2002	Toomey	D694,884 S	12/2013	Mooradian et al.
			D695,402 S	12/2013	Dacosta et al.
			8,652,142 B2	2/2014	Geissler
			8,657,820 B2	2/2014	Kubiak et al.
			D701,303 S	3/2014	Cook

(56)

References Cited

U.S. PATENT DOCUMENTS

8,672,945 B2	3/2014	Lavallee et al.	2005/0075641 A1	4/2005	Singhatat et al.	
8,696,716 B2	4/2014	Kartalian et al.	2005/0101961 A1	5/2005	Huebner et al.	
8,702,715 B2	4/2014	Ammann et al.	2005/0149042 A1	7/2005	Metzger	
D705,929 S	5/2014	Frey	2005/0228389 A1	10/2005	Stiernborg	
8,715,363 B2	5/2014	Ratron et al.	2005/0251147 A1	11/2005	Novak	
8,728,084 B2	5/2014	Berelsman et al.	2005/0267482 A1	12/2005	Hyde	
8,758,354 B2	6/2014	Habegger et al.	2005/0273112 A1	12/2005	Mcnamara	
8,764,760 B2	7/2014	Metzger et al.	2006/0122597 A1 *	6/2006	Jones	A61B 17/7083
8,764,763 B2	7/2014	Wong et al.				606/279
8,771,279 B2	7/2014	Philippon et al.	2006/0129163 A1	6/2006	Mcguire	
8,777,948 B2	7/2014	Bernsteiner	2006/0206044 A1	9/2006	Simon	
8,784,427 B2	7/2014	Fallin et al.	2006/0217733 A1	9/2006	Plassky et al.	
8,784,457 B2	7/2014	Graham	2006/0229621 A1	10/2006	Cadmus	
8,795,286 B2	8/2014	Sand et al.	2006/0235383 A1	10/2006	Hollawell	
8,801,727 B2	8/2014	Chan et al.	2006/0241607 A1	10/2006	Myerson et al.	
8,808,303 B2	8/2014	Stemniski et al.	2006/0241608 A1	10/2006	Myerson et al.	
8,828,012 B2	9/2014	May et al.	2006/0264961 A1	11/2006	Murray-Brown	
8,858,602 B2	10/2014	Weiner et al.	2007/0010818 A1	1/2007	Stone et al.	
8,882,778 B2	11/2014	Ranft	2007/0055233 A1	3/2007	Brinker	
8,882,816 B2	11/2014	Kartalian et al.	2007/0123857 A1	5/2007	Deffenbaugh et al.	
8,888,785 B2	11/2014	Ammann et al.	2007/0233138 A1	10/2007	Figuerola et al.	
D720,456 S	12/2014	Dacosta et al.	2007/0265634 A1	11/2007	Weinstein	
8,900,247 B2	12/2014	Tseng et al.	2007/0276383 A1	11/2007	Rayhack	
8,906,026 B2	12/2014	Ammann et al.	2008/0009863 A1	1/2008	Bond et al.	
8,945,132 B2	2/2015	Play et al.	2008/0015603 A1	1/2008	Collazo	
8,998,903 B2	4/2015	Price et al.	2008/0039850 A1	2/2008	Rowley et al.	
8,998,904 B2	4/2015	Zeetser et al.	2008/0091197 A1	4/2008	Coughlin	
9,023,052 B2	5/2015	Lietz et al.	2008/0140081 A1	6/2008	Heavener et al.	
9,044,250 B2	6/2015	Olsen et al.	2008/0147073 A1	6/2008	Ammann et al.	
9,060,822 B2	6/2015	Wright et al.	2008/0172054 A1	7/2008	Claypool et al.	
9,078,710 B2	7/2015	Thoren et al.	2008/0195215 A1	8/2008	Morton	
9,089,376 B2	7/2015	Medoff et al.	2008/0208252 A1	8/2008	Holmes	
9,101,421 B2	8/2015	Blacklidge	2008/0262500 A1	10/2008	Collazo	
9,107,715 B2	8/2015	Blitz et al.	2008/0269908 A1	10/2008	Warburton	
9,113,920 B2	8/2015	Ammann et al.	2008/0288004 A1	11/2008	Schendel	
D740,424 S	10/2015	Dacosta et al.	2009/0036893 A1	2/2009	Kartalian et al.	
D765,844 S	9/2016	Dacosta	2009/0036931 A1	2/2009	Pech et al.	
D766,434 S	9/2016	Dacosta	2009/0054899 A1	2/2009	Ammann et al.	
D766,437 S	9/2016	Dacosta	2009/0093849 A1	4/2009	Grabowski	
D766,438 S	9/2016	Dacosta	2009/0105767 A1	4/2009	Reiley	
D766,439 S	9/2016	Dacosta	2009/0118733 A1	5/2009	Orsak et al.	
9,452,057 B2	9/2016	Dacosta et al.	2009/0187189 A1	7/2009	Mirza et al.	
9,522,023 B2	11/2016	Haddad et al.	2009/0198244 A1	8/2009	Leibel	
9,592,084 B2	3/2017	Grant	2009/0198279 A1	8/2009	Zhang et al.	
9,622,805 B2	4/2017	Santrock et al.	2009/0216089 A1	8/2009	Davidson	
9,750,538 B2	9/2017	Soffiatti et al.	2009/0222047 A1	9/2009	Graham	
9,770,272 B2	9/2017	Thoren et al.	2009/0254092 A1	10/2009	Albiol Llorach	
9,785,747 B2	10/2017	Geebelen	2009/0254126 A1	10/2009	Orbay et al.	
9,924,969 B2	3/2018	Triplett et al.	2009/0287309 A1	11/2009	Walch et al.	
9,936,994 B2	4/2018	Smith et al.	2010/0030283 A1 *	2/2010	King	A61B 17/7082
9,980,760 B2	5/2018	Dacosta et al.				606/104
10,028,750 B2	7/2018	Rose	2010/0069910 A1	3/2010	Tasselman	
10,064,631 B2	9/2018	Dacosta et al.	2010/0121334 A1	5/2010	Couture et al.	
10,159,499 B2	12/2018	Dacosta et al.	2010/0130981 A1	5/2010	Richards	
10,292,713 B2	5/2019	Fallin et al.	2010/0152782 A1	6/2010	Stone et al.	
10,327,829 B2	6/2019	Dacosta et al.	2010/0168799 A1	7/2010	Schumer	
10,376,268 B2	8/2019	Fallin et al.	2010/0185245 A1	7/2010	Paul et al.	
10,470,779 B2	11/2019	Fallin et al.	2010/0249779 A1	9/2010	Hotchkiss et al.	
10,524,808 B1	1/2020	Hissong et al.	2010/0256687 A1	10/2010	Neufeld et al.	
10,779,867 B2	9/2020	Penzimer et al.	2010/0318088 A1	12/2010	Warne et al.	
10,939,939 B1	3/2021	Gil et al.	2010/0324556 A1	12/2010	Tyber et al.	
D945,610 S *	3/2022	Wilson	2011/0009865 A1	1/2011	Orfaly	
			2011/0093084 A1	4/2011	Morton	
			2011/0118739 A1	5/2011	Tyber et al.	
			2011/0178524 A1	7/2011	Lawrence et al.	
			2011/0245835 A1	10/2011	Dodds et al.	
			2011/0288550 A1	11/2011	Orbay et al.	
			2011/0301648 A1	12/2011	Lofthouse et al.	
11,304,705 B2	4/2022	Fallin et al.	2012/0016426 A1	1/2012	Robinson	
2002/0099381 A1	7/2002	Maroney	2012/0065689 A1	3/2012	Prasad et al.	
2002/0107519 A1	8/2002	Dixon et al.	2012/0078258 A1	3/2012	Lo et al.	
2002/0165552 A1	11/2002	Duffner	2012/0123420 A1	5/2012	Toniball	
2002/0198531 A1	12/2002	Millard et al.	2012/0123484 A1	5/2012	Lietz et al.	
2004/0010259 A1	1/2004	Keller et al.	2012/0130376 A1	5/2012	Loring et al.	
2004/0039394 A1	2/2004	Conti et al.	2012/0130382 A1	5/2012	Iannotti et al.	
2004/0097946 A1	5/2004	Dietzel et al.	2012/0130383 A1	5/2012	Budoff	
2004/0138669 A1	7/2004	Horn	2012/0184961 A1	7/2012	Johannaber	
2005/0004676 A1	1/2005	Schon et al.	2012/0185056 A1	7/2012	Warburton	
2005/0059978 A1	3/2005	Sherry et al.	2012/0191199 A1	7/2012	Raemisch	
2005/0070909 A1	3/2005	Egger et al.				

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0239045 A1 9/2012 Li
 2012/0253350 A1 10/2012 Anthony et al.
 2012/0265301 A1 10/2012 Demers et al.
 2012/0277745 A1 11/2012 Lizée
 2012/0303033 A1 11/2012 Weiner et al.
 2012/0330135 A1 12/2012 Millahn et al.
 2013/0012949 A1 1/2013 Fallin et al.
 2013/0035694 A1 2/2013 Grimm et al.
 2013/0085499 A1 4/2013 Lian
 2013/0085502 A1 4/2013 Harrold
 2013/0096563 A1 4/2013 Meade et al.
 2013/0131821 A1 5/2013 Cachia
 2013/0150900 A1 6/2013 Haddad et al.
 2013/0150903 A1 6/2013 Vincent
 2013/0158556 A1 6/2013 Jones et al.
 2013/0165936 A1 6/2013 Myers
 2013/0165938 A1 6/2013 Chow et al.
 2013/0172942 A1 7/2013 Wright et al.
 2013/0184714 A1 7/2013 Kaneyama et al.
 2013/0190765 A1 7/2013 Harris et al.
 2013/0190766 A1 7/2013 Harris et al.
 2013/0204259 A1 8/2013 Zajac
 2013/0226248 A1 8/2013 Hatch et al.
 2013/0226252 A1 8/2013 Mayer
 2013/0231668 A1 9/2013 Olsen et al.
 2013/0237987 A1 9/2013 Graham
 2013/0237989 A1 9/2013 Bonutti
 2013/0267956 A1 10/2013 Terrill et al.
 2013/0310836 A1 11/2013 Raub et al.
 2013/0325019 A1 12/2013 Thomas et al.
 2013/0325076 A1 12/2013 Palmer et al.
 2013/0331845 A1 12/2013 Horan et al.
 2013/0338785 A1 12/2013 Wong
 2014/0005672 A1 1/2014 Edwards et al.
 2014/0025127 A1 1/2014 Richter
 2014/0039501 A1 2/2014 Schickendantz et al.
 2014/0039561 A1 2/2014 Weiner et al.
 2014/0046387 A1 2/2014 Waizenegger
 2014/0074099 A1 3/2014 Vigneron et al.
 2014/0074101 A1 3/2014 Collazo
 2014/0094861 A1 4/2014 Fallin
 2014/0094924 A1 4/2014 Hacking et al.
 2014/0135775 A1 5/2014 Maxson et al.
 2014/0163563 A1 6/2014 Reynolds et al.
 2014/0171953 A1 6/2014 Gonzalvez et al.
 2014/0180342 A1 6/2014 Lowery et al.
 2014/0188139 A1 7/2014 Fallin et al.
 2014/0194884 A1 7/2014 Martin et al.
 2014/0194999 A1 7/2014 Orbay et al.
 2014/0207144 A1 7/2014 Lee et al.
 2014/0228899 A1 8/2014 Thoren et al.
 2014/0243825 A1 8/2014 Yapp et al.
 2014/0249537 A1 9/2014 Wong et al.
 2014/0257308 A1 9/2014 Johannaber
 2014/0257509 A1 9/2014 Dacosta et al.
 2014/0276815 A1 9/2014 Riccione
 2014/0276853 A1 9/2014 Long et al.
 2014/0277176 A1 9/2014 Buchanan et al.
 2014/0277214 A1 9/2014 Helenbolt et al.
 2014/0288562 A1 9/2014 Von Zubern et al.
 2014/0296995 A1 10/2014 Reiley et al.
 2014/0303621 A1 10/2014 Gerold et al.
 2014/0336658 A1 11/2014 Luna et al.
 2014/0343555 A1 11/2014 Russi et al.
 2014/0350561 A1 11/2014 Dacosta et al.
 2015/0032168 A1 1/2015 Orsak et al.
 2015/0045801 A1 2/2015 Axelson, Jr. et al.
 2015/0045839 A1 2/2015 Dacosta et al.
 2015/0051650 A1 2/2015 Verstreken et al.
 2015/0057667 A1 2/2015 Ammann et al.
 2015/0066094 A1 3/2015 Anderson et al.
 2015/0112446 A1 4/2015 Melamed et al.
 2015/0119944 A1 4/2015 Geldwert
 2015/0142064 A1 5/2015 Perez et al.
 2015/0150608 A1 6/2015 Sammarco

2015/0182273 A1 7/2015 Stemniski et al.
 2015/0223851 A1 8/2015 Hill et al.
 2015/0245858 A1 9/2015 Weiner et al.
 2016/0015426 A1 1/2016 Dayton
 2016/0022315 A1 1/2016 Soffiatti et al.
 2016/0135858 A1 5/2016 Dacosta et al.
 2016/0151165 A1 6/2016 Fallin et al.
 2016/0175089 A1 6/2016 Fallin et al.
 2016/0192950 A1 7/2016 Dayton et al.
 2016/0192970 A1 7/2016 Dayton et al.
 2016/0199076 A1 7/2016 Fallin et al.
 2016/0213384 A1 7/2016 Fallin et al.
 2016/0235414 A1 8/2016 Hatch et al.
 2016/0242791 A1 8/2016 Fallin et al.
 2016/0256204 A1 9/2016 Patel et al.
 2016/0270800 A1 9/2016 Sanders
 2016/0324532 A1 11/2016 Montoya et al.
 2016/0354127 A1 12/2016 Lundquist et al.
 2017/0014143 A1 1/2017 Dayton et al.
 2017/0014173 A1 1/2017 Smith et al.
 2017/0042598 A1 2/2017 Santrock et al.
 2017/0042599 A1 2/2017 Bays et al.
 2017/0079669 A1 3/2017 Bays et al.
 2017/0143511 A1 5/2017 Cachia
 2017/0164989 A1 6/2017 Weiner et al.
 2018/0132868 A1 5/2018 Dacosta et al.
 2018/0344334 A1 12/2018 Kim et al.
 2019/0350598 A1 11/2019 Jacobson
 2020/0015856 A1 1/2020 Treace et al.
 2020/0060731 A1* 2/2020 Richelsoph A61B 17/7074
 2020/0253641 A1 8/2020 Treace et al.
 2021/0236180 A1* 8/2021 DeCarbo A61B 17/7291
 2021/0244443 A1 8/2021 Coyne et al.
 2022/0211387 A1* 7/2022 Perler A61B 17/66

FOREIGN PATENT DOCUMENTS

CA 2854997 A1 5/2013
 CH 695846 A5 9/2006
 CN 2930668 Y 8/2007
 CN 201558162 U 8/2010
 CN 201572172 U 9/2010
 CN 201586060 U 9/2010
 CN 201912210 U 8/2011
 CN 101237835 B 11/2012
 CN 202801773 U 3/2013
 CN 103462675 A 12/2013
 CN 103505276 A 1/2014
 CN 203458450 U 3/2014
 CN 102860860 B 5/2014
 CN 203576647 U 5/2014
 CN 104490460 A 4/2015
 CN 104510523 A 4/2015
 CN 104523327 A 4/2015
 CN 104546102 A 4/2015
 CN 204379413 U 6/2015
 CN 204410951 U 6/2015
 CN 204428143 U 7/2015
 CN 204428144 U 7/2015
 CN 204428145 U 7/2015
 CN 204446081 U 7/2015
 DE 202006010241 U1 3/2007
 DE 102007053058 B3 4/2009
 EP 685206 B1 9/2000
 EP 1508316 B1 5/2007
 EP 1897509 B1 7/2009
 EP 2124772 A1 12/2009
 EP 2124832 B1 8/2012
 EP 2632349 A1 9/2013
 EP 2665428 A1 11/2013
 EP 2742878 A1 6/2014
 EP 2750617 A1 7/2014
 EP 2849684 A1 3/2015
 EP 2932925 A1 10/2015
 EP 2624764 B1 12/2015
 EP 3023068 A2 5/2016
 FR 2362616 A1 3/1978
 FR 2764183 B1 11/1999
 FR 2953120 B1 1/2012

(56)

References Cited

FOREIGN PATENT DOCUMENTS

FR	3030221	A1	6/2016
GB	2154143	A	9/1985
GB	2154144	A	9/1985
GB	2334214	B	1/2003
IN	200903719	P1	6/2009
IN	200904479	P2	5/2010
IN	140/DELNP/2012	P1	2/2013
IN	2004/KOLNP/2013	P2	11/2013
JP	S635739	A	1/1988
JP	2004174265	A	6/2004
JP	2006158972	A	6/2006
JP	4134243	B2	8/2008
JP	4162380	B2	10/2008
JP	2011092405	A	5/2011
JP	2011523889	A	8/2011
JP	4796943	B2	10/2011
JP	5466647	B2	4/2014
JP	2014511207	A	5/2014
JP	2014521384	A	8/2014
JP	6628875	B2	11/2014
KR	100904142	B1	6/2009
MD	756	Z	11/2014
RU	2098036	C1	12/1997
RU	2195892	C2	1/2003
RU	2320287	C1	3/2008
RU	2321366	C2	4/2008
RU	2321369	C1	4/2008
RU	2346663	C2	2/2009
RU	2412662	C1	2/2011
SU	1333328	A2	8/1987
WO	0166022	A1	9/2001
WO	03075775	A1	9/2003
WO	2004089227	A2	10/2004
WO	2005122923	A1	12/2005
WO	2008051064	A1	5/2008
WO	2009029798	A1	3/2009
WO	2009032101	A2	3/2009
WO	2011037885	A1	3/2011
WO	2012029008	A1	3/2012
WO	2013090392	A1	6/2013
WO	2013134387	A1	9/2013
WO	2013169475	A1	11/2013
WO	2014020561	A1	2/2014
WO	2014022055	A1	2/2014
WO	2014035991	A1	3/2014
WO	2014085882	A1	6/2014
WO	2014147099	A1	9/2014
WO	2014152219	A2	9/2014
WO	2014152535	A1	9/2014
WO	2014177783	A1	11/2014
WO	2014200017	A1	12/2014
WO	2015094409	A1	6/2015
WO	2015105880	A1	7/2015
WO	2015127515	A2	9/2015
WO	2016134160	A1	8/2016

OTHER PUBLICATIONS

Simpson et al., "Computer-Assisted Distraction Osteogenesis By Ilizarov's Method," International Journal of Medical Robots and Computer Assisted Surgery, vol. 4, No. 4, Dec. 2008, pp. 310-320, (Abstract Only).

Small Bone External Fixation System, Acumed, Surgical Technique, Effective date Sep. 2014, 8 pages.

"Smith & Nephew scores a Hat-Trick with its entry into the high-growth hammer toe repair market," Smith & Nephew, Jul. 31, 2014, 2 pages.

Smith et al., "Opening Wedge Osteotomies for Correction of Hallux Valgus: A Review of Wedge Plate Fixation," Foot and Ankle Specialist, vol. 2, No. 6, Dec. 2009, pp. 277-282.

Sokoloff, "Lapidus Procedure," Textbook of Bunion Surgery, Chapter 15, 1981, pp. 277-287.

"Speed Continuous Active Compression Implant," BioMedical Enterprises, Inc., A120-029 Rev. 3, 2013, 4 pages.

Stableloc External Fixation System, Acumed, Product Overview, Effective date Sep. 2015, 4 pages.

Stahl et al., "Derotation Of Post-Traumatic Femoral Deformities By Closed Intramedullary Sawing," Injury, vol. 37, No. 2, Feb. 2006, pp. 145-151, (Abstract Only).

Stamatis et al., "Mini Locking Plate as "Medial Buttress" for Oblique Osteotomy for Hallux Valgus," Foot & Ankle International, vol. 31, No. 10, Oct. 2010, pp. 920-922.

Stewart, "Use for BME Speed Nitinol Staple Fixation for the Lapidus Procedure," date unknown, 1 page.

Talbot et al., "Assessing Sesamoid Subluxation: How Good is the AP Radiograph?," Foot and Ankle International, vol. 19, No. 8, Aug. 1998, pp. 547-554.

TempFix Spanning the Ankle Joint Half Pin and Transfixing Pin Techniques, Biomet Orthopedics, Surgical Technique, 2012, 16 pages.

Toth et al., "The Effect of First Ray Shortening in the Development of Metatarsalgia in the Second Through Fourth Rays After Metatarsal Osteotomy," Foot & Ankle International, vol. 28, No. 1, Jan. 2007, pp. 61-63.

Tricot et al., "3D-corrective osteotomy using surgical guides for posttraumatic distal humeral deformity," Acta Orthopaedica Belgica, vol. 78, No. 4, 2012, pp. 538-542.

"Visionaire: Patient Matched Cutting Blocks Surgical Procedure," Smith & Nephew, Inc., 2009, 2 pages.

Vitek et al., "Die Behandlung des Hallux rigidus mit Cheilektomie und Akin-Moberg-Osteotomie unter Verwendung einer neuen Schnittlehre und eines neuen Schraubensystems," Orthopadische Praxis, vol. 44, Nov. 2008, pp. 563-566, including English Abstract on p. 564.

Vitek, "Neue Techniken in der Fußchirurgie Das V-tek-System," ABW Wissenschaftsverlag GmbH, 2009, 11 pages, including English Abstract.

Walker et al., "The Role of First Ray Insufficiency in the Development of Metatarsalgia," Foot and Ankle Clinics, vol. 24, No. 4, Dec. 2019, published online: Sep. 5, 2019, pp. 641-648.

Weber et al., "Use of the First Ray Splay Test to Assess Transverse Plane Instability Before First Metatarsocuneiform Fusion," The Journal of Foot and Ankle Surgery, vol. 45, No. 4, Jul./Aug. 2006, pp. 278-282.

Weber et al., "A Simple System For Navigation Of Bone Alignment Osteotomies Of The Tibia," International Congress Series, vol. 1268, Jan. 2004, pp. 608-613, (Abstract Only).

Weil et al., "Anatomic Plantar Plate Repair Using the Weil Metatarsal Osteotomy Approach," Foot & Ankle Specialist, vol. 4, No. 3, 2011, pp. 145-150.

Wendl et al., "Navigation in der Knieendoprothetik," OP-Journal, vol. 17, 2002, pp. 22-27, including English Abstract.

Whipple et al., "Zimmer Herbert Whipple Bone Screw System: Surgical Techniques for Fixation of Scaphoid and Other Small Bone Fractures," Zimmer, 2003, 59 pages.

Wienke et al., "Bone Stimulation For Nonunions: What the Evidence Reveals," Podiatry Today, vol. 24, No. 9, Sep. 2011, pp. 52-57.

Wukich et al., "Hypermobility of the First Tarsometatarsal Joint," Foot and Ankle Clinics, vol. 10, No. 1, Mar. 2005, pp. 157-166.

Yacki et al., "Compression Forces of Internal and External Ankle Fixation Devices with Simulated Bone Resorption," Foot and Ankle International, vol. 31, No. 1, Jan. 2010, pp. 76-85, (Abstract Only).

Yasuda et al., "Proximal Supination Osteotomy of the First Metatarsal for Hallux Valgus," Foot and Ankle International, vol. 36, No. 6, Jun. 2015, pp. 696-704.

Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 41 pages.

Prior Art Publications, Exhibit A of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 3 pages. Claim Chart for Fishco, "Making the Lapidus Easy," The Podiatry Institute (Apr. 2014), Exhibit B1 of Defendant Fusion Orthopedics

(56)

References Cited

OTHER PUBLICATIONS

LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 97 pages.

Claim Chart for Fishco, "A Straightforward Guide to the Lapidus Bunionectomy," HMP Global (Sep. 6, 2013), Exhibit B2 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 67 pages.

Claim Chart for Groves, "Functional Position Joint Sectioning: Pre-Load Method for Lapidus Arthrodesis," Update 2015: Proceedings of the Annual Meeting of the Podiatry Institute, Chpt. 6, pp. 23-29 (Apr. 2015), Exhibit B3 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 151 pages.

Claim Chart for Mote, "First Metatarsal-Cuneiform Arthrodesis for the Treatment of First Ray Pathology: A Technical Guide," The Journal Foot & Ankle Surgery (Sep. 1, 2009), Exhibit B5 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 21 pages.

Claim Chart for U.S. Pat. No. 10,376,268 to Fallin et al., entitled "Indexed Tri-Planar Osteotomy Guide and Method," issued Aug. 13, 2019, Exhibit B6 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 155 pages.

Claim Chart for U.S. Pat. No. 8,282,645 to Lawrence et al., entitled "Metatarsal Bone Implant Cutting Guide," issued Jan. 18, 2010, Exhibit B7 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 76 pages.

Claim Chart for U.S. Pat. No. 9,452,057 to Dacosta et al., entitled "Bone Implants and Cutting Apparatuses and Methods," issued Apr. 8, 2011, Exhibit B8 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 110 pages.

Obviousness Chart, Exhibit C of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 153 pages.

Dayton et al., "Principles of Management of Growth Plate Fractures in the Foot and Ankle," Clinics in Podiatric Medicine and Surgery, Pediatric Foot Deformities, Oct. 2013, 17 pages.

Dayton et al., "Observed Changes in Radiographic Measurements of the First Ray after Frontal and Transverse Plane Rotation of the Hallux: Does the Hallux Drive the Metatarsal in a Bunion Deformity?," The Journal of Foot and Ankle Surgery, Article in Press, 2014, 4 pages.

Dayton et al., "Comparison of Complications for Internal and External Fixation for Charcot Reconstruction: A Systematic Review," The Journal of Foot and Ankle Surgery, Article in Press, 2015, 4 pages.

Dayton et al., "A new triplanar paradigm for bunion management," Lower Extremity Review, Apr. 2015, 9 pages.

Dayton et al., "American College of Foot and Ankle Surgeons' Clinical Consensus Statement: Perioperative Prophylactic Antibiotic Use in Clean Elective Foot Surgery," The Journal of Foot and Ankle Surgery, Article in Press, 2015, 7 pages.

Dayton et al., "Complications of Metatarsal Suture Techniques for Bunion Correction: A Systematic Review of the Literature," The Journal of Foot and Ankle Surgery, Article in Press, 2015, 3 pages.

DeCarbo et al., "The Weil Osteotomy: A Refresher," Techniques in Foot and Ankle Surgery, vol. 13, No. 4, Dec. 2014, pp. 191-198.

DeCarbo et al., "Resurfacing Interpositional Arthroplasty for Degenerative Joint Disease of the First Metatarsalphalangeal Joint," Podiatry Management, Jan. 2013, pp. 137-142.

DeCarbo et al., "Locking Plates: Do They Prevent Complications?," Podiatry Today, Apr. 2014, 7 pages.

De Geer et al., "A New Measure of Tibial Sesamoid Position in Hallux Valgus in Relation to the Coronal Rotation of the First Metatarsal in CT Scans," Foot and Ankle International, Mar. 26, 2015, 9 pages.

DiDomenico et al., "Correction of Frontal Plane Rotation of Sesamoid Apparatus during the Lapidus Procedure: A Novel Approach," The Journal of Foot and Ankle Surgery, vol. 53, 2014, pp. 248-251.

DiDomenico et al., "Lapidus Bunionectomy: First Metatarsal-Cuneiform Arthrodesis," McGlamry's Comprehensive Textbook of Foot and Ankle Surgery, Fourth Edition, vol. 1, Chapter 31, 2013, 24 pages.

Dobbe et al., "Patient-Tailored Plate For Bone Fixation And Accurate 3D Positioning In Corrective Osteotomy," Medical and Biological Engineering and Computing, vol. 51, No. 1-2, Feb. 2013, pp. 19-27, (Abstract Only).

Doty et al., "Hallux valgus and hypermobility of the first ray: facts and fiction," International Orthopaedics, vol. 37, 2013, pp. 1655-1660.

Easley et al., "Current Concepts Review: Hallux Valgus Part I: Pathomechanics, Clinical Assessment, and Nonoperative Management," Foot and Ankle International, vol. 28, No. 5, May 2007, pp. 654-659.

Easley et al., "Current Concepts Review: Hallux Valgus Part II: Operative Treatment," Foot and Ankle International, vol. 28, No. 6, Jun. 2007, pp. 748-758.

Easley et al., "What is the Best Treatment for Hallux Valgus?," Evidence-Based Orthopaedics—The Best Answers to Clinical Questions, Chapter 73, 2009, pp. 479-491.

EBI Extra Small Rail Fixator, Biomet Trauma, retrieved Dec. 19, 2014, from the Internet: <<http://footandanklefixation.com/product/biomet-trauma-ebi-extra-small-rail-fixator>>, 7 pages.

Eustace et al., "Hallux valgus, first metatarsal pronation and collapse of the medial longitudinal arch—a radiological correlation," Skeletal Radiology, vol. 23, 1994, pp. 191-194.

Fallin et al., US Provisional Application Entitled Indexed Tri-Planar Osteotomy Guide and Method, U.S. Appl. No. 62/118,378, filed Feb. 19, 2015, 62 pages.

Feilmeier et al., "Reduction of Intermetatarsal Angle after First Metatarsophalangeal Joint Arthrodesis in Patients with Hallux Valgus," The Journal of Foot and Ankle Surgery, vol. 53, 2014, pp. 29-31.

Fishco, "A Straightforward Guide To The Lapidus Bunionectomy," Podiatry Today, Retrieved online from <<https://www.hmpglobal-learningnetwork.com/site/podiatry/blogged/straightforward-guide-lapidus-bunionectomy>>, dated Sep. 6, 2013, 5 pages.

Feilmeier et al., "Incidence of Surgical Site Infection in the Foot and Ankle with Early Exposure and Showering of Surgical Sites: A Prospective Observation," The Journal of Foot and Ankle Surgery, vol. 53, 2014, pp. 173-175.

Fishco, "Making the Lapidus Easy," The Podiatry Institute, Update 2014, Chapter 14, 2014, pp. 91-93.

Fleming et al., "Results of Modified Lapidus Arthrodesis Procedure Using Medial Eminence as an Interpositional Autograft," The Journal of Foot & Ankle Surgery, vol. 50, 2011, pp. 272-275.

"Foot and Ankle Instrument Set," Smith & Nephew, 2013, 2 pages.

Fuhrmann, "Arthrodesis of the First Tarsometatarsal Joint for Correction of the Advanced Splayfoot Accompanied by a Hallux Valgus," Operative Orthopaedie und Traumatologie, No. 2, 2005, pp. 195-210.

"Futura Forefoot Implant Arthroplasty Products," Tornier, Inc., 2008, 12 pages.

Galli et al., "Enhanced Lapidus Arthrodesis: Crossed Screw Technique With Middle Cuneiform Fixation Further Reduces Sagittal Mobility," The Journal of Foot & Ankle Surgery, vol. 54, vol. 3, May/Jun. 2015, published online: Nov. 21, 2014, pp. 437-440.

Garthwait, "Accu-Cut System Facilitates Enhanced Precision," Podiatry Today, vol. 18, No. 6, Jun. 2005, 6 pages.

Gerard et al., "The Modified Lapidus Procedure," Orthopedics, vol. 31, No. 3, Mar. 2008, 7 pages.

Giannoudis et al., "Hallux Valgus Correction," Practical Procedures in Elective Orthopaedic Surgery, Pelvis and Lower Extremity, Chapter 38, 2012, 22 pages.

Gonzalez Del Pino et al., "Variable Angle Locking Intercarpal Fusion System for Four-Corner Arthrodesis: Indications and Surgical Technique," Journal of Wrist Surgery, vol. 1, No. 1, Aug. 2012, pp. 73-78.

(56)

References Cited

OTHER PUBLICATIONS

Gotte, "Entwicklung eines Assistenzrobotersystems für die Knieendoprothetik," Forschungsberichte, Technische Universität München, 165, 2002, 11 pages, including partial English Translation.

Gregg et al., "Plantar plate repair and Weil osteotomy for metatarsophalangeal joint instability," *Foot and Ankle Surgery*, vol. 13, 2007, pp. 116-121.

Greiner, "The Jargon of Pedal Movements," *Foot & Ankle International*, vol. 28, No. 1, Jan. 2007, pp. 109-125.

Grondal et al., "A Guide Plate for Accurate Positioning of First Metatarsophalangeal Joint during Fusion," *Operative Orthopädie Und Traumatologie*, vol. 16, No. 2, 2004, pp. 167-178 (Abstract Only).

Groves, "Operative Report," St. Tammany Parish Hospital, Date of Procedure, Mar. 26, 2014, 2 pages.

Groves, "Functional Position Joint Sectioning: Pre-Load Method for Lapidus Arthrodesis," *The Podiatry Institute*, Update 2015, Chapter 6, 2015, pp. 23-29.

Hardy et al., "Observations on Hallux Valgus," *The Journal of Bone and Joint Surgery*, vol. 33B, No. 3, Aug. 1951, pp. 376-391.

Hatch et al., "Triplane Hallux Abducto Valgus Classification," *The Journal of Foot & Ankle Surgery*, vol. 57, No. 5, Sep./Oct. 2018, published online: May 18, 2018, pp. 972-981.

"Hat-Trick Lesser Toe Repair System," Smith & Nephew, Brochure, Aug. 2014, 12 pages.

"Hat-Trick Lesser Toe Repair System, Foot and Ankle Technique Guide, Metatarsal Shortening Osteotomy Surgical Technique," Smith & Nephew, 2014, 16 pages.

Hetherington et al., "Evaluation of surgical experience and the use of an osteotomy guide on the apical angle of an Austin osteotomy," *The Foot*, vol. 18, 2008, pp. 159-164.

Hirao et al., "Computer assisted planning and custom-made surgical guide for malunited pronation deformity after first metatarsophalangeal joint arthrodesis in rheumatoid arthritis: A case report," *Computer Aided Surgery*, vol. 19, Nos. 1-3, 2014, pp. 13-19.

"Hoffmann II Compact External Fixation System," Stryker, Brochure, Literature No. 5075-1-500, 2006, 12 pages.

"Hoffmann II Micro Lengthener," Stryker, Operative Technique, Literature No. 5075-2-002, 2008, 12 pages.

"Hoffmann Small System External Fixator Orthopedic Instruments," Stryker, retrieved Dec. 19, 2014, from the Internet: <http://www.alibaba.com/product-detail/Stryker-Hoffmann-Small-System-External-Fixator_1438850129.html>, 3 pages.

Holmes, Jr., "Correction of the Intermetatarsal Angle Component of Hallux Valgus Using Fiberwire-Attached Endo-buttons," *Revista Internacional de Ciencias Podologicas*, vol. 6, No. 2, 2012, pp. 73-79.

Integra, "Integra Large Qwix Positioning and Fixation Screw, Surgical Technique," 2012, 16 pages.

Kilmartin et al., "Combined rotation scarf and Akin osteotomies for hallux valgus: a patient focused 9 year follow up of 50 patients," *Journal of Foot and Ankle Research*, vol. 3, No. 2, 2010, 12 pages.

Kim et al., "A Multicenter Retrospective Review of Outcomes for Arthrodesis, Hemi-Metallic Joint Implant, and Resectional Arthroplasty in the Surgical Treatment of End-Stage Hallux Rigidus," *The Journal of Foot and Ankle Surgery*, vol. 51, 2012, pp. 50-56.

Kim et al., "A New Measure of Tibial Sesamoid Position in Hallux Valgus in Relation to the Coronal Rotation of the First Metatarsal in CT Scans," *Foot and Ankle International*, vol. 36, No. 8, 2015, pp. 944-952.

"Lag Screw Target Bow," Stryker Leibinger GmbH & Co. KG, Germany 2004, 8 pages.

Langan et al., "Maintenance of Correction of the Modified Lapidus Procedure With a First Metatarsal to Intermediate Cuneiform Cross-Screw Technique," *Foot & Ankle International*, vol. 41, No. 4, Apr. 1, 2020, published online: Dec. 26, 2019, pp. 426-436.

"Lapidus Pearls: Gaining Joint Exposure to Decrease Non-Union," Youtube, Retrieved online from <<https://www.youtube.com/watch?v=-jqJyE7pj-Y>>, dated Nov. 2, 2009, 3 pages.

Lapidus, "The Author's Bunion Operation From 1931 to 1959," *Clinical Orthopaedics*, vol. 16, 1960, pp. 119-135.

Lee et al., "Technique Tip: Lateral Soft-Tissue Release for Correction of Hallux Valgus Through a Medial Incision Using A Dorsal Flap Over the First Metatarsal," *Foot & Ankle International*, vol. 28, No. 8, Aug. 2007, pp. 949-951.

Li et al., "Evolution of Thinking of the Lapidus Procedure and Fixation," *Foot and Ankle Clinics*, vol. 25, No. 1, Mar. 2020, published online: Dec. 16, 2019, pp. 18 pages.

Lieske et al., "Implantation einer Sprunggelenkttotalendo-prothese vom Typ Salto 2," *Operative Orthopädie und Traumatologie*, vol. 26, No. 4, 2014, pp. 401-413, including English Abstract on p. 403.

Lopez et al., "Metatarsalgia: Assessment Algorithm and Decision Making," *Foot and Ankle Clinics*, vol. 24, No. 4, Dec. 2019, published online: Sep. 25, 2019, pp. 561-569.

MAC (Multi Axial Correction) Fixation System, Biomet Trauma, retrieved Dec. 19, 2014, from the Internet: <<http://footandanklefixation.com/product/biomet-trauma-mac-multi-axial-correction-fixation-system>>, 7 pages.

Magin, "Computernavigierter Gelenkersatz am Knie mit dem Orthopilot," *Operative Orthopädie und Traumatologie*, vol. 22, No. 1, 2010, pp. 63-80, including English Abstract on p. 64.

Magin, "Die belastungsstabile Lapidus-Arthrodesse bei Hallux-valgus-Deformität mittels IVP-Plattenfixateur (V-TEK-System)," *Operative Orthopädie und Traumatologie*, vol. 26, No. 2, 2014, pp. 184-195, including English Abstract on p. 186.

Michelangelo Bunion System, Surgical Technique, Instratek Incorporated, publication date unknown, 4 pages.

Mini Joint Distractor, Arthrex, retrieved Dec. 19, 2014, from the Internet: <<http://www.arthrex.com/foot-ankle/mini-joint-distractor/products>>, 2 pages.

MiniRail System, Small Bone Innovations, Surgical Technique, 2010, 24 pages.

Miyake et al., "Three-Dimensional Corrective Osteotomy for Malunited Diaphyseal Forearm Fractures Using Custom-Made Surgical Guides Based on Computer Simulation," *JBJS Essential Surgical Techniques*, vol. 2, No. 4, 2012, 11 pages.

Mizuno et al., "Detorsion Osteotomy of the First Metatarsal Bone in Hallux Valgus," *Japanese Orthopaedic Association*, Tokyo, 1956; 30:813-819.

Modular Rail System: External Fixator, Smith & Nephew, Surgical Technique, 2013, 44 pages.

Monnich et al., "A Hand Guided Robotic Planning System for Laser Osteotomy in Surgery," *World Congress on Medical Physics and Biomedical Engineering* vol. 25/6: Surgery, Minimal Invasive Interventions, Endoscopy and Image Guided Therapy, Sep. 7-12, 2009, pp. 59-62, (Abstract Only).

Moore et al., "Effect Of Ankle Flexion Angle On Axial Alignment Of Total Ankle Replacement," *Foot and Ankle International*, vol. 31, No. 12, Dec. 2010, pp. 1093-1098, (Abstract Only).

Mortier et al., "Axial Rotation of the First Metatarsal Head in a Normal Population and Hallux Valgus Patients," *Orthopaedics and Traumatology: Surgery and Research*, vol. 98, 2012, pp. 677-683.

Mote et al., "First Metatarsal-Cuneiform Arthrodesis for the Treatment of First Ray Pathology: A Technical Guide," *JFAS Techniques Guide*, vol. 48, No. 5, Sep./Oct. 2009, pp. 593-601.

Myerson, "Cuneiform-Metatarsal Arthrodesis," *The Foot and Ankle*, Chapter 9, 1997, pp. 107-117.

Nagy et al., "The AO Ulnar Shortening Osteotomy System Indications and Surgical Technique," *Journal of Wrist Surgery*, vol. 3, No. 2, 2014, pp. 91-97.

NexFix from Nexa Orthopedics, MetaFix I from Merete Medical, Inc. and The BioPro Lower Extremities from BioPro, found in *Foot & Ankle International Journal*, vol. 28, No. 1, Jan. 2007, 4 pages.

Odenbring et al., "A guide instrument for high tibial osteotomy," *Acta Orthopaedica Scandinavica*, vol. 60, No. 4, 1989, pp. 449-451.

Okuda et al., "The Shape of the Lateral Edge of the First Metatarsal Head as a Risk Factor for Recurrence of Hallux Valgus," *The Journal of Bone and Joint Surgery*, vol. 89, 2007, pp. 2163-2172.

Okuda et al., "Proximal Metatarsal Osteotomy for Hallux Valgus: Comparison of Outcome for Moderate and Severe Deformities," *Foot and Ankle International*, vol. 29, No. 7, Jul. 2008, pp. 664-670.

(56)

References Cited

OTHER PUBLICATIONS

Okuda et al., "Postoperative Incomplete Reduction of the Sesamoids as a Risk Factor for Recurrence of Hallux Valgus," *The Journal of Bone and Joint Surgery*, vol. 91-A, No. 1, Jul. 2009, pp. 1637-1645.

Osher et al., "Accurate Determination of Relative Metatarsal Protrusion with a Small Intermetatarsal Angle: A Novel Simplified Method," *The Journal of Foot & Ankle Surgery*, vol. 53, No. 5, Sep./Oct. 2014, published online: Jun. 3, 2014, pp. 548-556.

Otsuki et al., "Developing a novel custom cutting guide for curved per-acetabular osteotomy," *International Orthopaedics (SICOT)*, vol. 37, 2013, pp. 1033-1038.

Patel et al., "Modified Lapidus Arthrodesis: Rate of Nonunion in 227 Cases," *The Journal of Foot & Ankle Surgery*, vol. 43, No. 1, Jan./Feb. 2004, pp. 37-42.

"Patient to Patient Precision, Accu-Cut, Osteotomy Guide System," *BioPro, Foot & Ankle International Journal*, vol. 23, No. 8, Aug. 2002, 2 pages.

Peters et al., "Flexor Hallucis Longus Tendon Laceration as a Complication of Total Ankle Arthroplasty," *Foot & Ankle International*, vol. 34, No. 1, 2013, pp. 148-149.

"Prophecy Inbone Preoperative Navigation Guides," *Wright Medical Technology, Inc.*, Nov. 2013, 6 pages.

Ray et al., "Multicenter Early Radiographic Outcomes of Triplanar Tarsometatarsal Arthrodesis With Early Weightbearing," *Foot & Ankle International*, vol. 40, No. 8, Aug. 1, 2019, published online: May 5, 2019, 7 pages.

"Rayhack Ulnar Shortening Generation II Low-Profile Locking System Surgical Technique," *Wright Medical Technology, Inc.*, Dec. 2013, 20 pages.

"Reconstructive Surgery of the Foot & Ankle," *The Podiatry Institute, Update 2015, Conference Program*, May 2015, 28 pages.

Rodriguez et al., "Ilizarov method of fixation for the management of pilon and distal tibial fractures in the compromised diabetic patient: A technique guide," *The Foot and Ankle Journal Online*, vol. 7, No. 2, 2014, 9 pages.

Rx-Fix Mini Rail External Fixator, *Wright Medical Technology, Brochure*, Aug. 15, 2014, 2 pages.

Saltzman et al., "Prospective Controlled Trial of Star Total Ankle Replacement Versus Ankle Fusion: Initial Results," *Foot & Ankle International*, vol. 30, No. 7, Jul. 2009, pp. 579-596.

Sammarco, "Surgical Strategies: Mau Osteotomy for Correction of Moderate and Severe Hallux Valgus Deformity," *Foot & Ankle International*, vol. 28, No. 7, Jul. 2007, pp. 857-864.

Sandhu et al., "Digital Arthrodesis With a One-Piece Memory Nitinol Intramedullary Fixation Device: A Retrospective Review," *Foot and Ankle Specialist*, vol. 6, No. 5, Oct. 2013, pp. 364-366.

Scanlan et al., "Technique Tip: Subtalar Joint Fusion Using a Parallel Guide and Double Screw Fixation," *The Journal of Foot and Ankle Surgery*, vol. 49, Issue 3, May-Jun. 2010, pp. 305-309, (Abstract Only).

Schon et al., "Cuneiform—Metatarsal Arthrodesis for Hallux Valgus," *The Foot and Ankle, Second Edition*, Chapter 8, 2002, pp. 99-117.

Scranton Jr. et al., "Anatomic Variations in the First Ray: Part I. Anatomic Aspects Related to Bunions Surgery," *Clinical Orthopaedics and Related Research*, vol. 151, Sep. 1980, pp. 244-255.

Shurnas et al., "Proximal Metatarsal Opening Wedge Osteotomy," *Operative Techniques in Foot and Ankle Surgery*, Section I, Chapter 13, 2011, pp. 73-78.

Siddiqui et al., "Fixation Of Metatarsal Fracture With Bone Plate In A Dromedary Heifer," *Open Veterinary Journal*, vol. 3, No. 1, 2013, pp. 17-20.

"Accu-Cut Osteotomy Guide System," *BioPro, Brochure*, Oct. 2018, 2 pages.

"Acumed Osteotomiesystem Operationstechnik," *Acumed*, 2014, 19 pages (including 3 pages English translation).

Albano et al., "Biomechanical Study of Transcortical or Transtrabecular Bone Fixation of Patellar Tendon Graft with Bioabsorbable Pins in ACL Reconstruction in Sheep," *Revista Brasileira de Ortopedia (Rev Bras Ortop.)* vol. 47, No. 1, 2012, pp. 43-49.

Alvine et al., "Peg and Dowel Fusion of the Proximal Interphalangeal Joint," *Foot & Ankle*, vol. 1, No. 2, 1980, pp. 90-94.

Anderson et al., "Uncemented Star Total Ankle Prostheses," *The Journal of Bone and Joint Surgery*, vol. 86(1, Suppl 2), Sep. 2004, pp. 103-111, (Abstract Only).

Arthrex, "Comprehensive Foot System," Retrieved online from <https://www.arthrex.com/resources/animation/BU3iaPvY6kO8bwFAwZF50Q/comprehensive-foot-system?referringTeam=foot_and_ankle>, dated Aug. 27, 2013, 3 pages.

Baravarian, "Why the Lapidus Procedure is Ideal for Bunions," *Podiatry Today*, Retrieved online from <<https://www.hmpglobal-learnhmpglobal.com/site/podipodi/article/5542>>, dated May 2006, 8 pages.

Bauer et al., "Offset-V Osteotomy of the First Metatarsal Shaft in Hallux Abducto Valgus," *McGlamry's Comprehensive Textbook of Foot and Ankle Surgery*, Fourth Edition, vol. 1, Chapter 29, 2013, 26 pages.

Bednarz et al., "Modified Lapidus Procedure for the Treatment of Hypermobile Hallux Valgus," *Foot & Ankle International*, vol. 21, No. 10, Oct. 2000, pp. 816-821.

Blomer, "Knieendoprothetik—Herstellerische Probleme und technologische Entwicklungen," *Orthopade*, vol. 29, 2000, pp. 688-696, including English Abstract on p. 689.

Boffeli et al., "Can We Abandon Saw Wedge Resection in Lapidus Fusion? A Comparative Study of Joint Preparation Techniques Regarding Correction of Deformity, Union Rate, and Preservation of First Ray Length," *The Journal of Foot and Ankle Surgery*, vol. 58, No. 6, Nov. 2019, published online: Sep. 25, 2019, pp. 1118-1124.

Bouaicha et al., "Fixation of Maximal Shift Scarf Osteotomy with Inside Out Plating: Technique Tip," *Foot & Ankle International*, vol. 32, No. 5, May 2011, pp. 567-569.

Carr et al., "Correctional Osteotomy for Metatarsus Primus Varus and Hallux Valgus," *The Journal of Bone and Joint Surgery*, vol. 50-A, No. 7, Oct. 1968, pp. 1353-1367.

Catanese et al., "Measuring Sesamoid Position in Hallux Valgus: When Is the Sesamoid Axial View Necessary," *Foot and Ankle Specialist*, 2014, 3 pages.

Claim Chart for Groves Public Use (Mar. 26, 2014), Exhibit B4 of Defendant Fusion Orthopedics LLC's Invalidity Contentions, No. CV-22-00490-PHX-SRB, US District Court for the District of Arizona, Aug. 27, 2022, 161 pages.

Coetzee et al., "Revision Hallux Valgus Correction," *Operative Techniques in Foot and Ankle Surgery*, Section I, Chapter 15, 2011, pp. 84-96.

Coetzee et al., "The Lapidus Procedure: A Prospective Cohort Outcome Study," *Foot & Ankle International*, vol. 25, No. 8, Aug. 2004, pp. 526-531.

Collan et al., "The biomechanics of the first metatarsal bone in hallux valgus: A preliminary study utilizing a weight bearing extremity CT," *Foot and Ankle Surgery*, vol. 19, 2013, pp. 155-161.

Conti et al., "Effect of the Modified Lapidus Procedure on Pronation of the First Ray in Hallux Valgus," *Foot & Ankle International*, Feb. 1, 2020, published online: Oct. 16, 2019, 8 pages.

Conti et al., "Effect of the Modified Lapidus Procedure for Hallux Valgus on Foot Width," *Foot & Ankle International*, Feb. 1, 2020, published online: Oct. 30, 2019, 6 pages.

Cottom, "Fixation of the Lapidus Arthrodesis with a Plantar Interfragmentary Screw and Medial Low Profile Locking Plate," *The Journal of Foot & Ankle Surgery*, vol. 51, 2012, pp. 517-522.

Coughlin, "Proximal Metatarsal Osteotomy and Distal Soft Tissue Reconstruction for Hallux Valgus in Juveniles," *Orthopaedics and Traumatology*, vol. 7, 1999, pp. 133-143.

Cruz et al., "Does Hallux Valgus Exhibit a Deformity Inherent to the First Metatarsal Bone?" *The Journal of Foot & Ankle Surgery*, vol. 58, No. 6, Nov. 2019, pp. 1210-1214.

D'Amico et al., "Motion of the First Ray: Clarification Through Investigation," *Journal of the American Podiatry Association*, vol. 69, No. 1, Jan. 1979, pp. 17-23.

Dahlgren et al., "First Tarsometatarsal Fusion Using Saw Preparation vs. Standard Preparation of the Joint: A Cadaver Study," *Foot & Ankle Orthopaedics*, vol. 4, No. 4, Oct. 2019, 2 pages.

(56)

References Cited

OTHER PUBLICATIONS

Dayton et al., "Comparison of the Mechanical Characteristics of a Universal Small Biplane Plating Technique Without Compression Screw and Single Anatomic Plate With Compression Screw," *The Journal of Foot & Ankle Surgery*, vol. 55, No. 3, May/Jun. 2016, published online: Feb. 9, 2016, pp. 567-571.

Dayton et al., "Evidence-Based Bunion Surgery: A Critical Examination of Current and Emerging Concepts and Techniques," Springer International Publishing, 2017, 254 pages.

Dayton et al., "Is Our Current Paradigm for Evaluation and Management of the Bunion Deformity Flawed? A Discussion of Procedure Philosophy Relative to Anatomy," *The Journal of Foot and Ankle Surgery*, vol. 54, 2015, pp. 102-111.

Dayton et al., "Observed Changes in Radiographic Measurements of the First Ray after Frontal and Transverse Plane Rotation of the Hallux: Does the Hallux Drive the Metatarsal in a Bunion Deformity?," *The Journal of Foot and Ankle Surgery*, vol. 53, 2014, pp. 584-587.

Dayton et al., "Relationship Of Frontal Plane Rotation Of First Metatarsal To Proximal Articular Set Angle And Hallux Alignment In Patients Undergoing Tarsometatarsal Arthrodesis For Hallux Abducto Valgus: A Case Series And Critical Review Of The Literature," *The Journal of Foot and Ankle Surgery*, vol. 52, No. 3, May/Jun. 2013, pp. 348-354.

Dayton et al., "Quantitative Analysis of the Degree of Frontal Rotation Required to Anatomically Align the First Metatarsal Phalangeal Joint During Modified Tarsal-Metatarsal Arthrodesis Without Capsular Balancing," *The Journal of Foot and Ankle Surgery*, 2015, pp. 1-6.

Dayton et al., "Observed Changes in Radiographic Measurements of the First Ray after Frontal Plane Rotation of the First Metatarsal in a Cadaveric Foot Model," *The Journal of Foot & Ankle Surgery*, vol. 53, 2014, pp. 274-278.

Dayton et al., "Relationship of Frontal Plane Rotation of First Metatarsal to Proximal Articular Set Angle and Hallux Alignment in Patients Undergoing Tarsometatarsal Arthrodesis for Hallux Abducto Valgus: A Case Series and Critical Review of the Literature," *The Journal of Foot & Ankle Surgery*, 2013, Article in Press, Mar. 1, 2013, 7 pages.

Dayton et al., "Biwinged Excision for Round Pedal Lesions," *The Journal of Foot and Ankle Surgery*, vol. 35, No. 3, 1996, pp. 244-249.

Dayton et al., "Medial Incision Approach to the First Metatarsophalangeal Joint," *The Journal of Foot and Ankle Surgery*, vol. 40, No. 6, Nov./Dec. 2001, pp. 414-417.

Dayton et al., "Reduction of the Intermetatarsal Angle after First Metatarsophalangeal Joint Arthrodesis in Patients with Moderate and Severe Metatarsus Primus Adductus," *The Journal of Foot and Ankle Surgery*, vol. 41, No. 5, Sep./Oct. 2002, pp. 316-319.

Dayton et al., "Use of the Z Osteotomy for Tailor Bunionectomy," *The Journal of Foot and Ankle Surgery*, vol. 42, No. 3, May/Jun. 2003, pp. 167-169.

Dayton et al., "Early Weightbearing After First Metatarsophalangeal Joint Arthrodesis: A Retrospective Observational Case Analysis," *The Journal of Foot and Ankle Surgery*, vol. 43, No. 3, May/Jun. 2004, pp. 156-159.

Dayton et al., "Dorsal Suspension Stitch: An Alternative Stabilization After Flexor Tenotomy for Flexible Hammer Digit Syndrome," *The Journal of Foot and Ankle Surgery*, vol. 48, No. 5, Sep./Oct. 2009, pp. 602-605.

Dayton et al., "The Extended Knee Hemilithotomy Position for Gastrocnemius Recession," *The Journal of Foot and Ankle Surgery*, vol. 49, 2010, pp. 214-216.

Dayton et al., "Hallux Varus as Complication of Foot Compartment Syndrome," *The Journal of Foot and Ankle Surgery*, vol. 50, 2011, pp. 504-506.

Dayton et al., "Measurement of Mid-Calcaneal Length on Plain Radiographs: Reliability of a New Method," *Foot and Ankle Specialist*, vol. 4, No. 5, Oct. 2011, pp. 280-283.

Dayton et al., "A User-Friendly Method of Pin Site Management for External Fixators," *Foot and Ankle Specialist*, Sep. 16, 2011, 4 pages.

Dayton et al., "Effectiveness of a Locking Plate in Preserving Midcalcaneal Length and Positional Outcome after Evans Calcaneal Osteotomy: A Retrospective Pilot Study," *The Journal of Foot and Ankle Surgery*, vol. 52, 2013, pp. 710-713.

Dayton et al., "Does Postoperative Showering or Bathing of a Surgical Site Increase the Incidence of Infection? A Systematic Review of the Literature," *The Journal of Foot and Ankle Surgery*, vol. 52, 2013, pp. 612-614.

Dayton et al., "Technique for Minimally Invasive Reduction of Calcaneal Fractures Using Small Bilateral External Fixation," *The Journal of Foot and Ankle Surgery*, Article in Press, 2014, 7 pages.

Dayton et al., "Clarification of the Anatomic Definition of the Bunion Deformity," *The Journal of Foot and Ankle Surgery*, vol. 53, 2014, pp. 160-163.

Dayton et al., "Observed Changes in Radiographic Measurements of the First Ray after Frontal Plane Rotation of the First Metatarsal in a Cadaveric Foot Model," *The Journal of Foot and Ankle Surgery*, Article in Press, 2014, 5 pages.

Dayton et al., "Observed Changes in First Metatarsal and Medial Cuneiform Positions after First Metatarsophalangeal Joint Arthrodesis," *The Journal of Foot and Ankle Surgery*, vol. 53, 2014, pp. 32-35.

Dayton et al., "Reduction of the Intermetatarsal Angle after First Metatarsal Phalangeal Joint Arthrodesis: A Systematic Review," *The Journal of Foot and Ankle Surgery*, Article in Press, 2014, 4 pages.

* cited by examiner

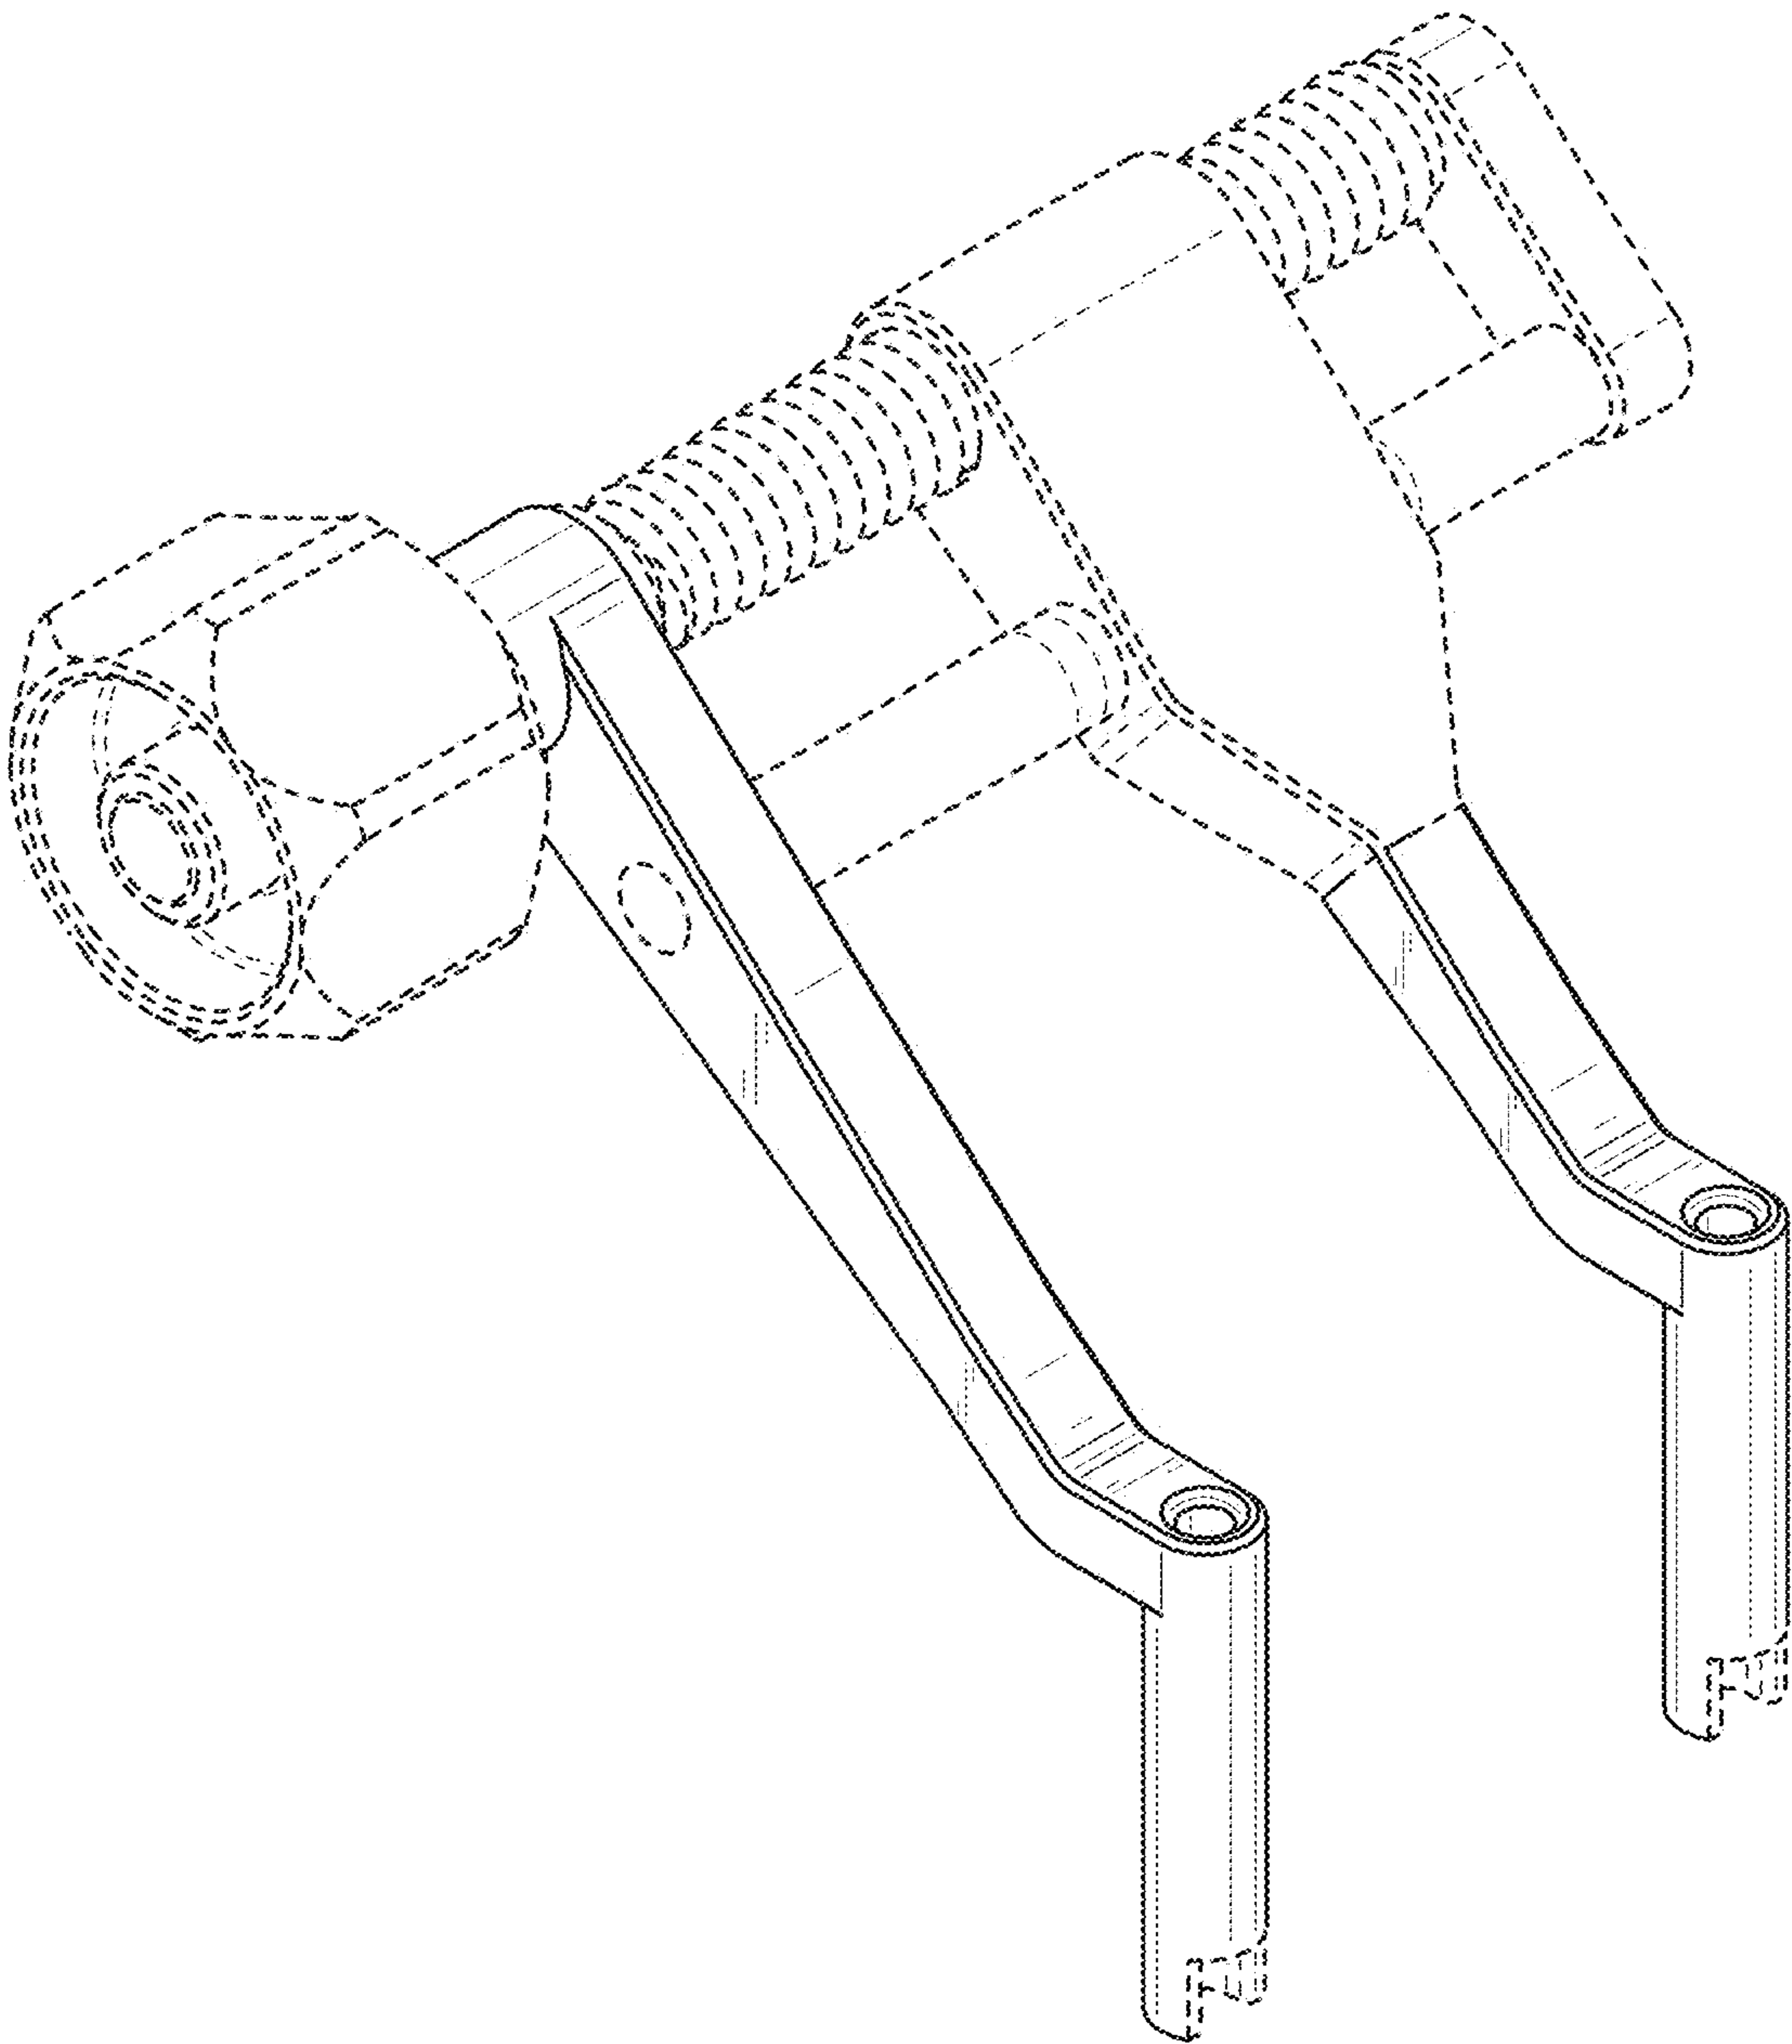


FIG. 1

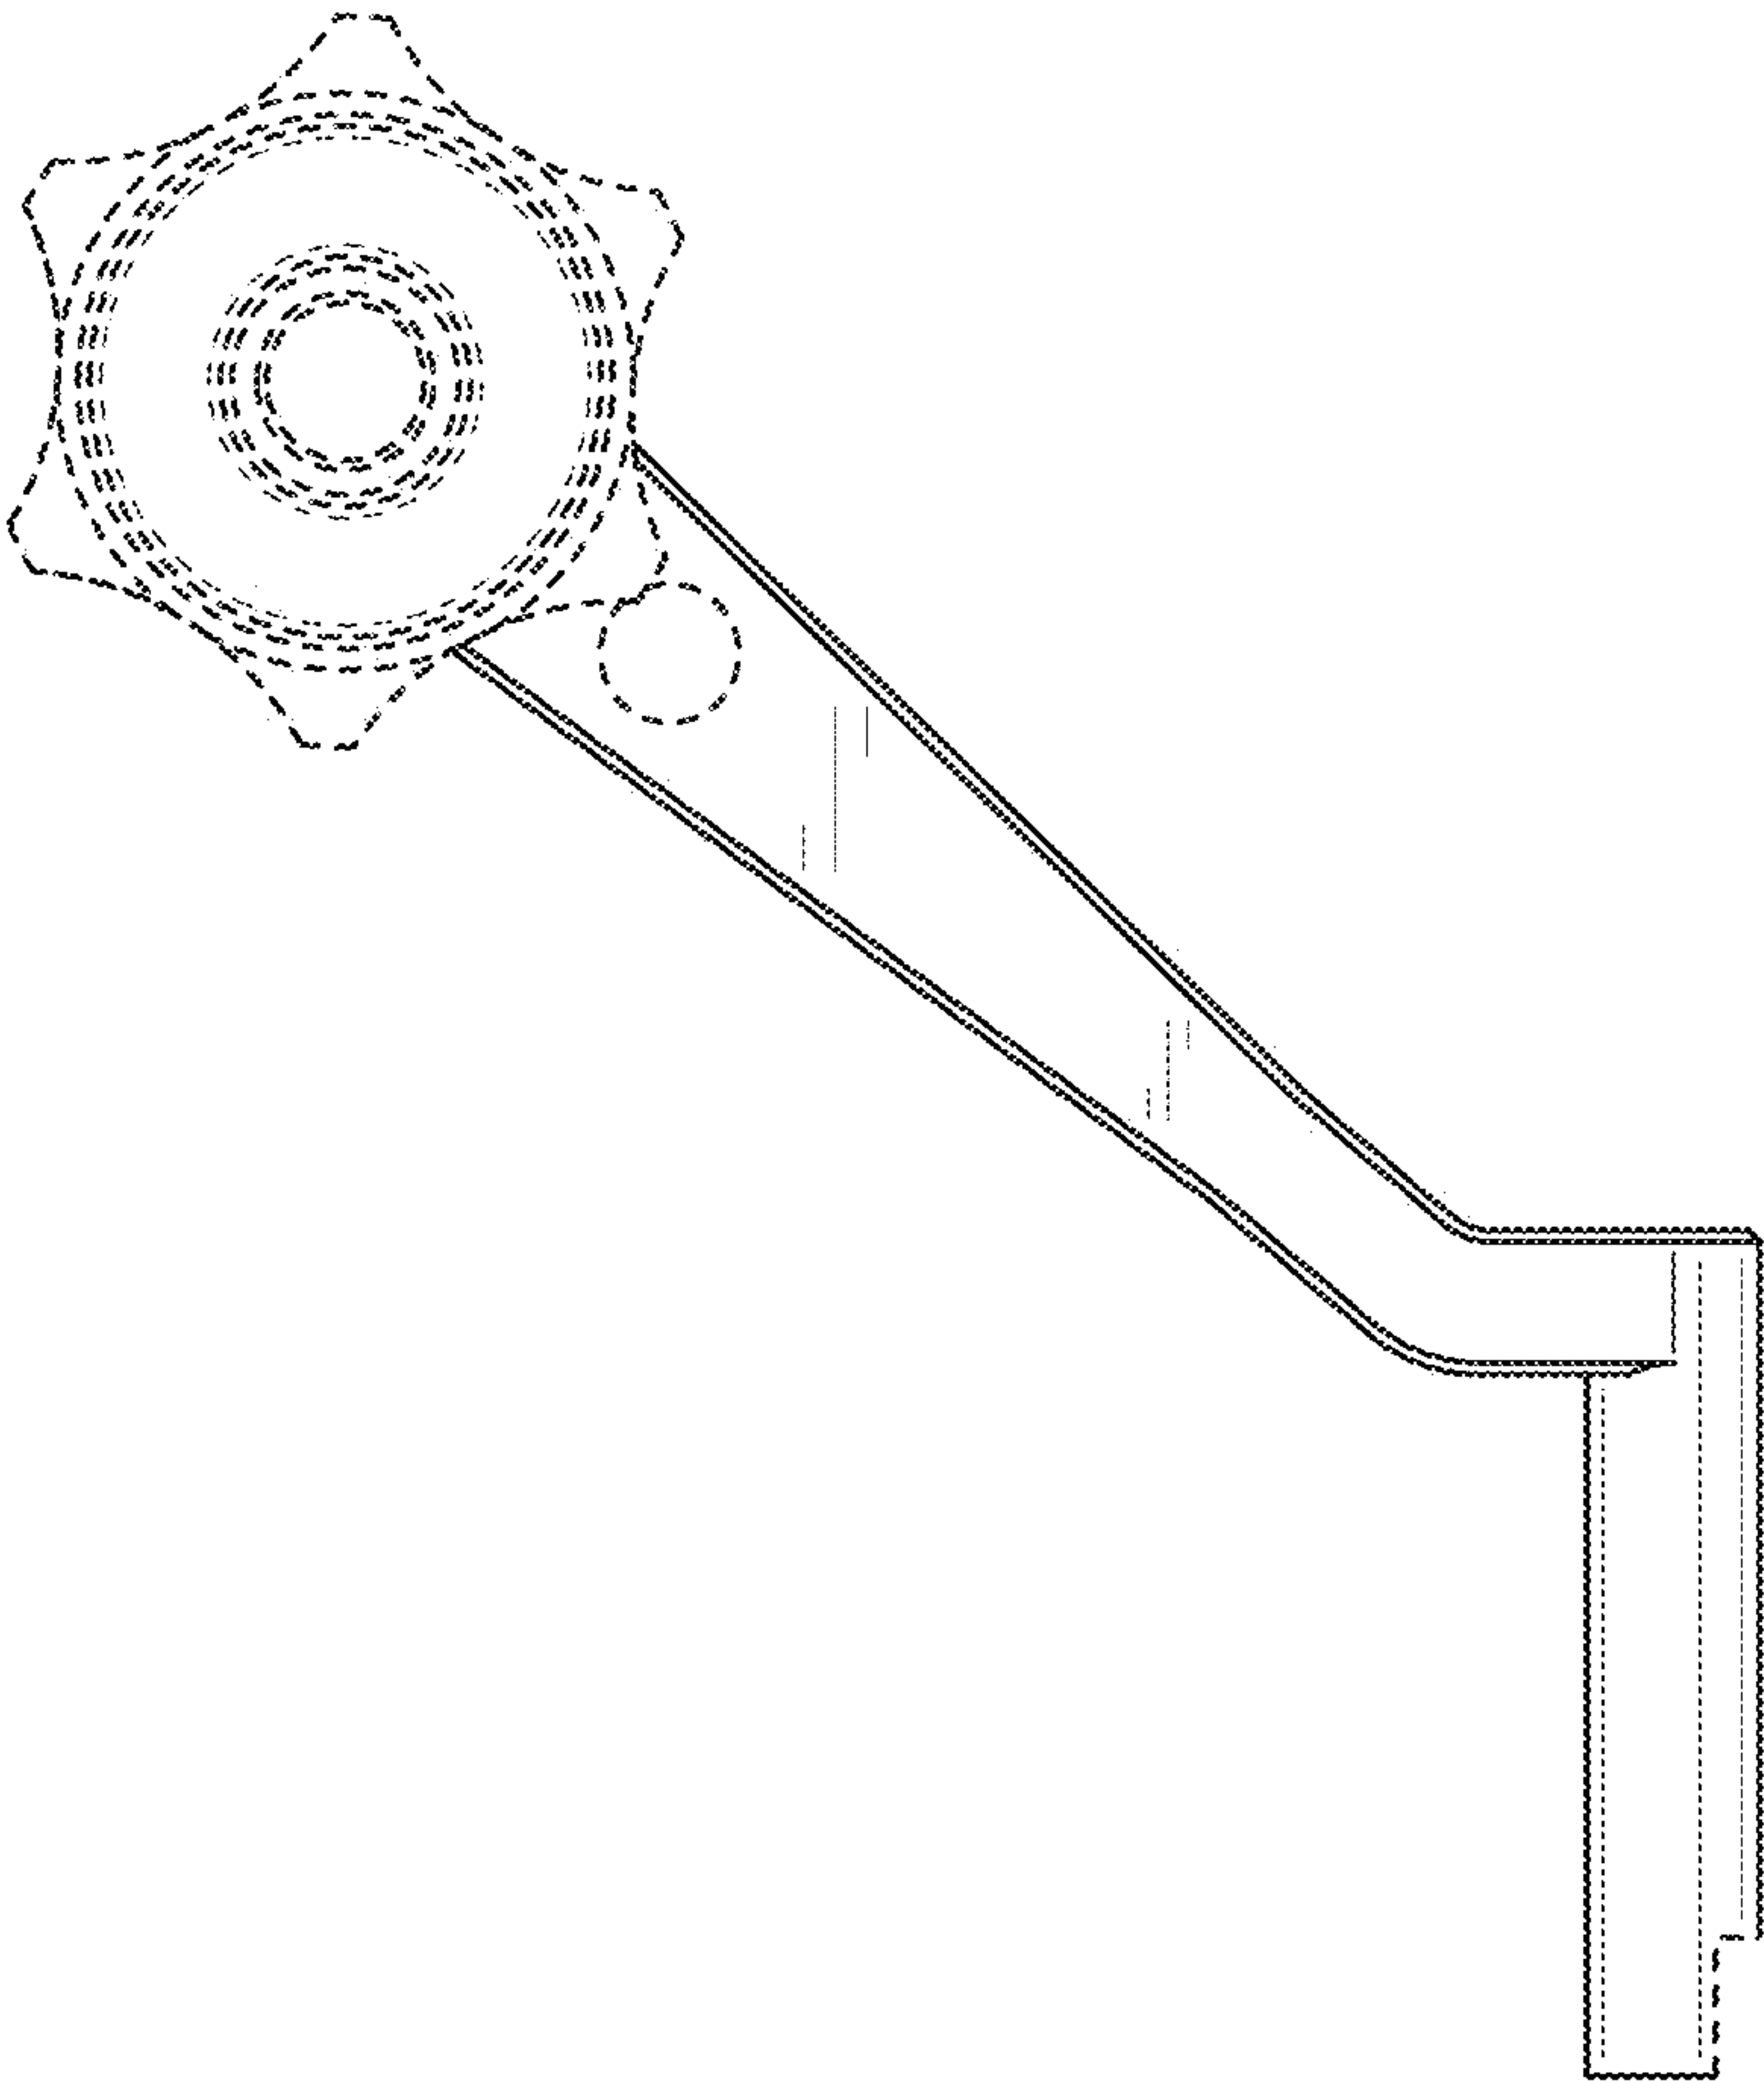


FIG. 2

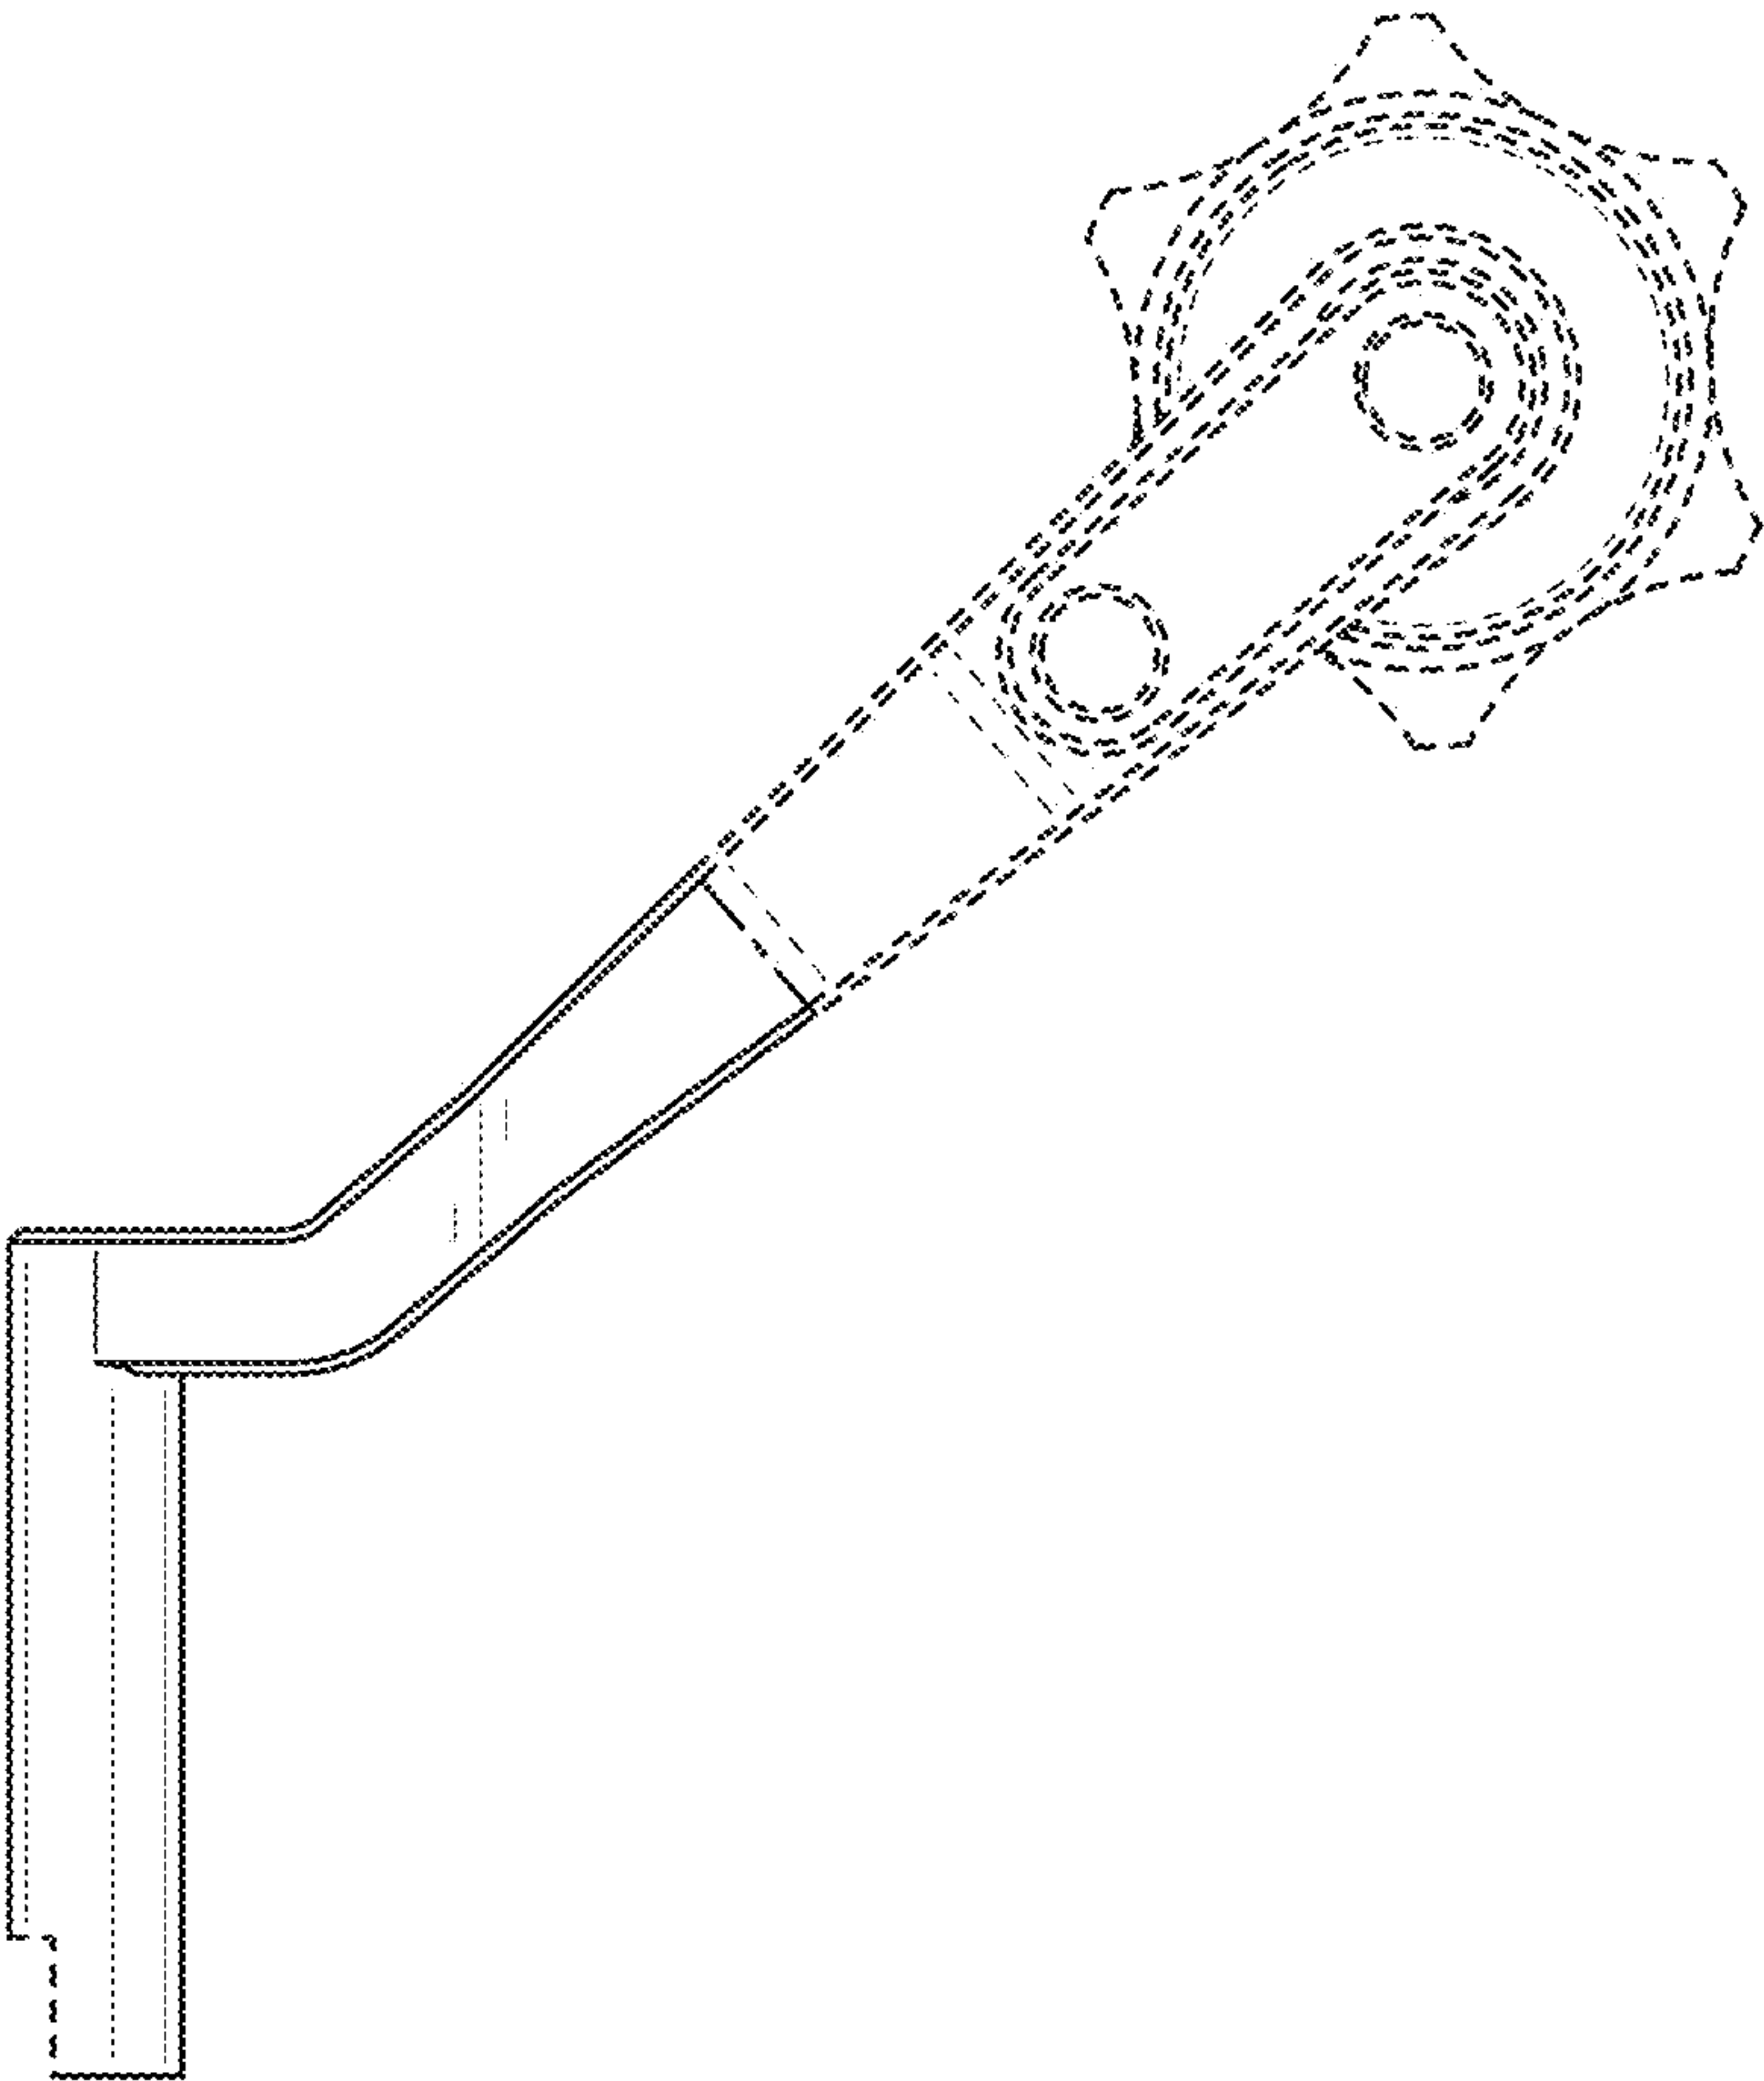


FIG. 3

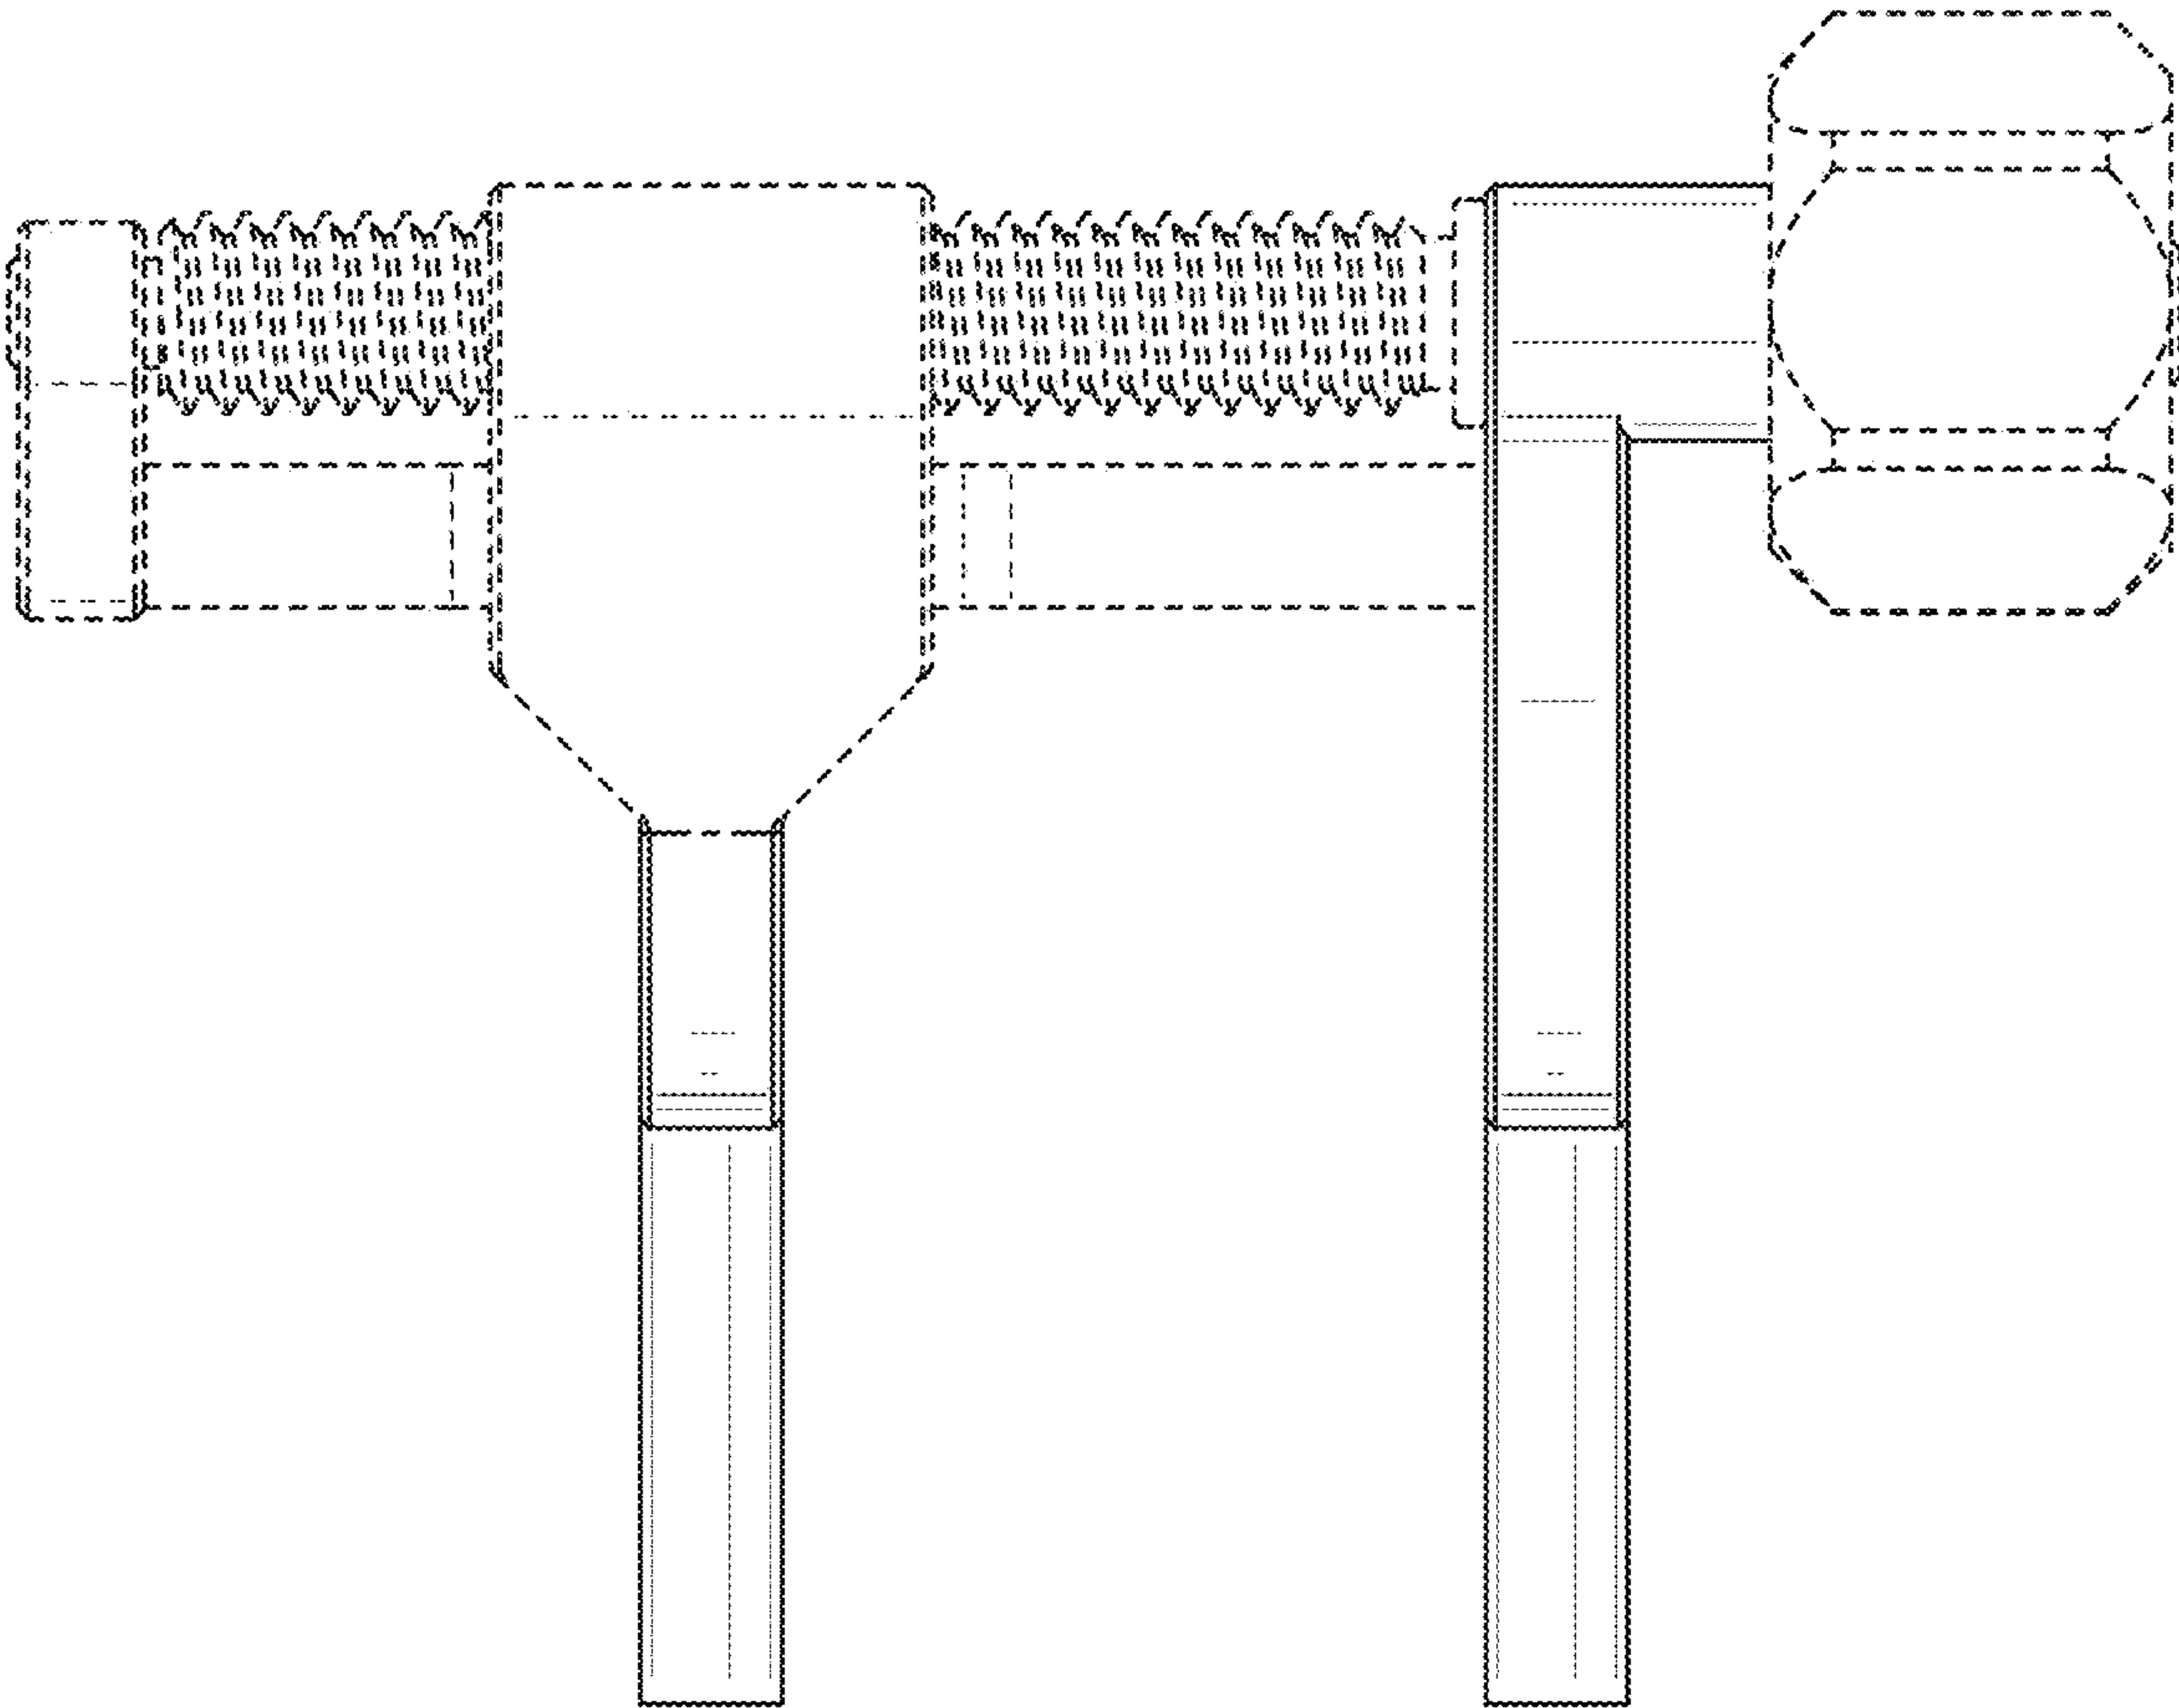


FIG. 4

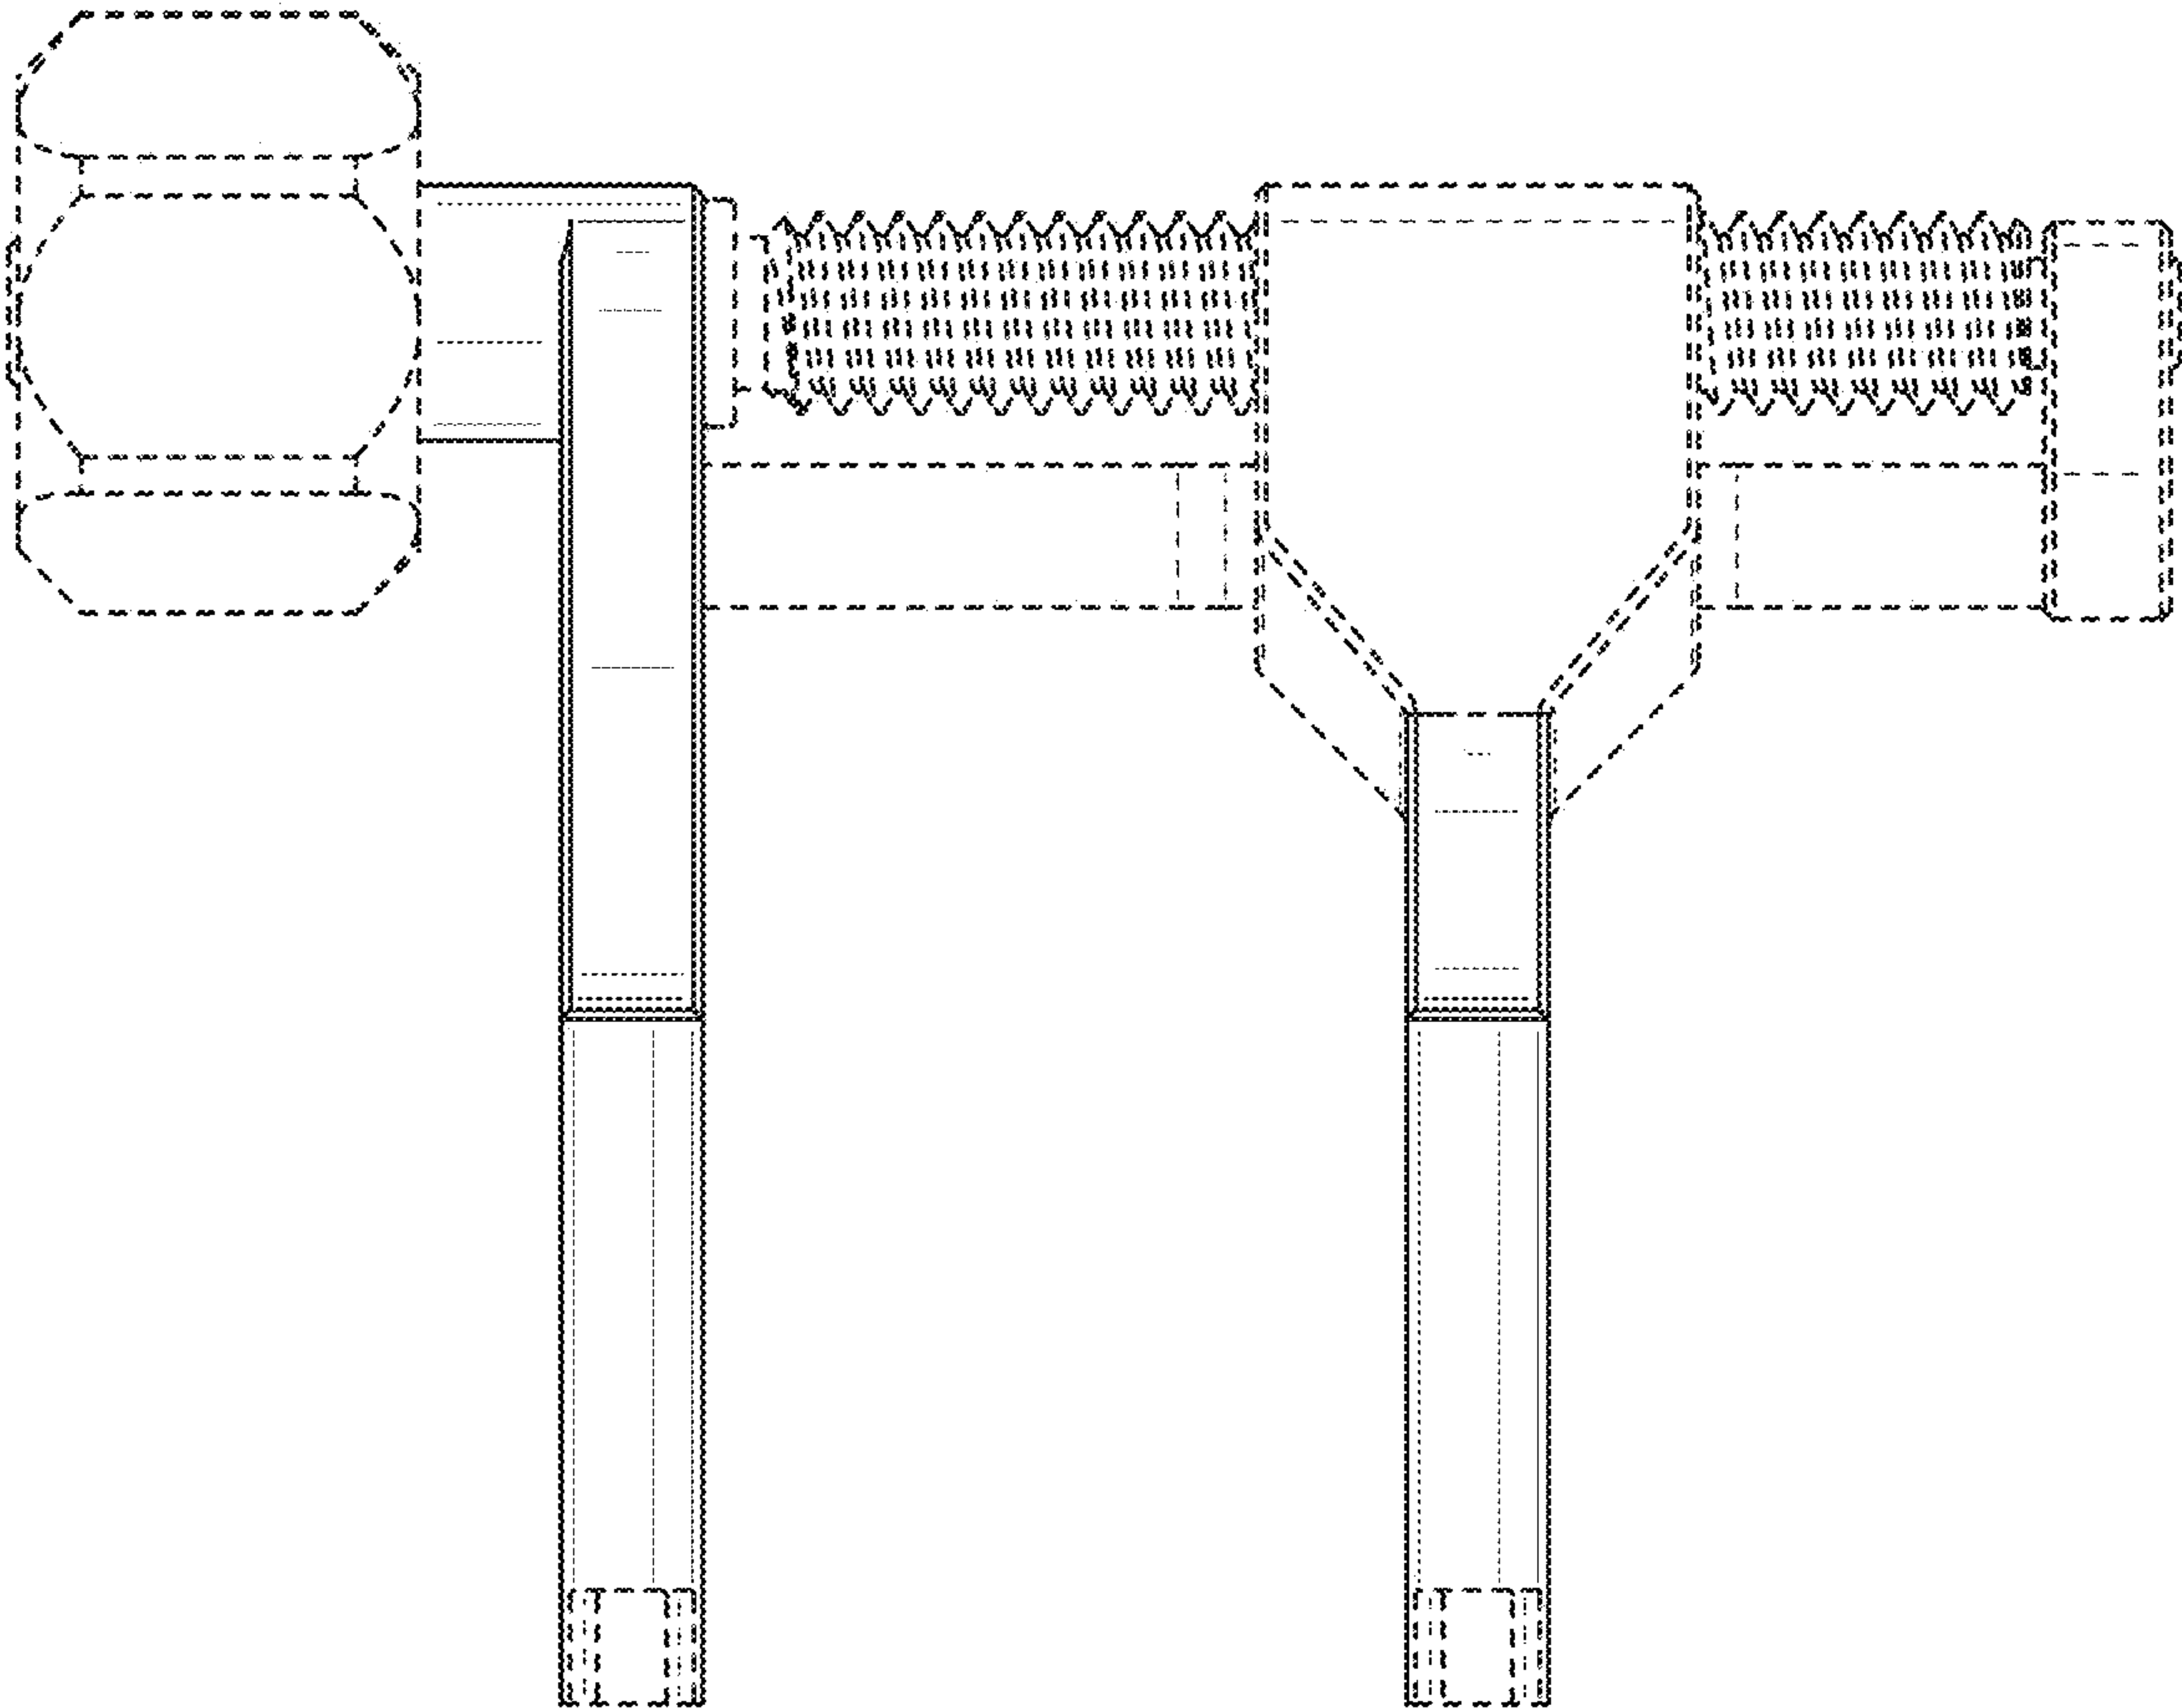


FIG. 5

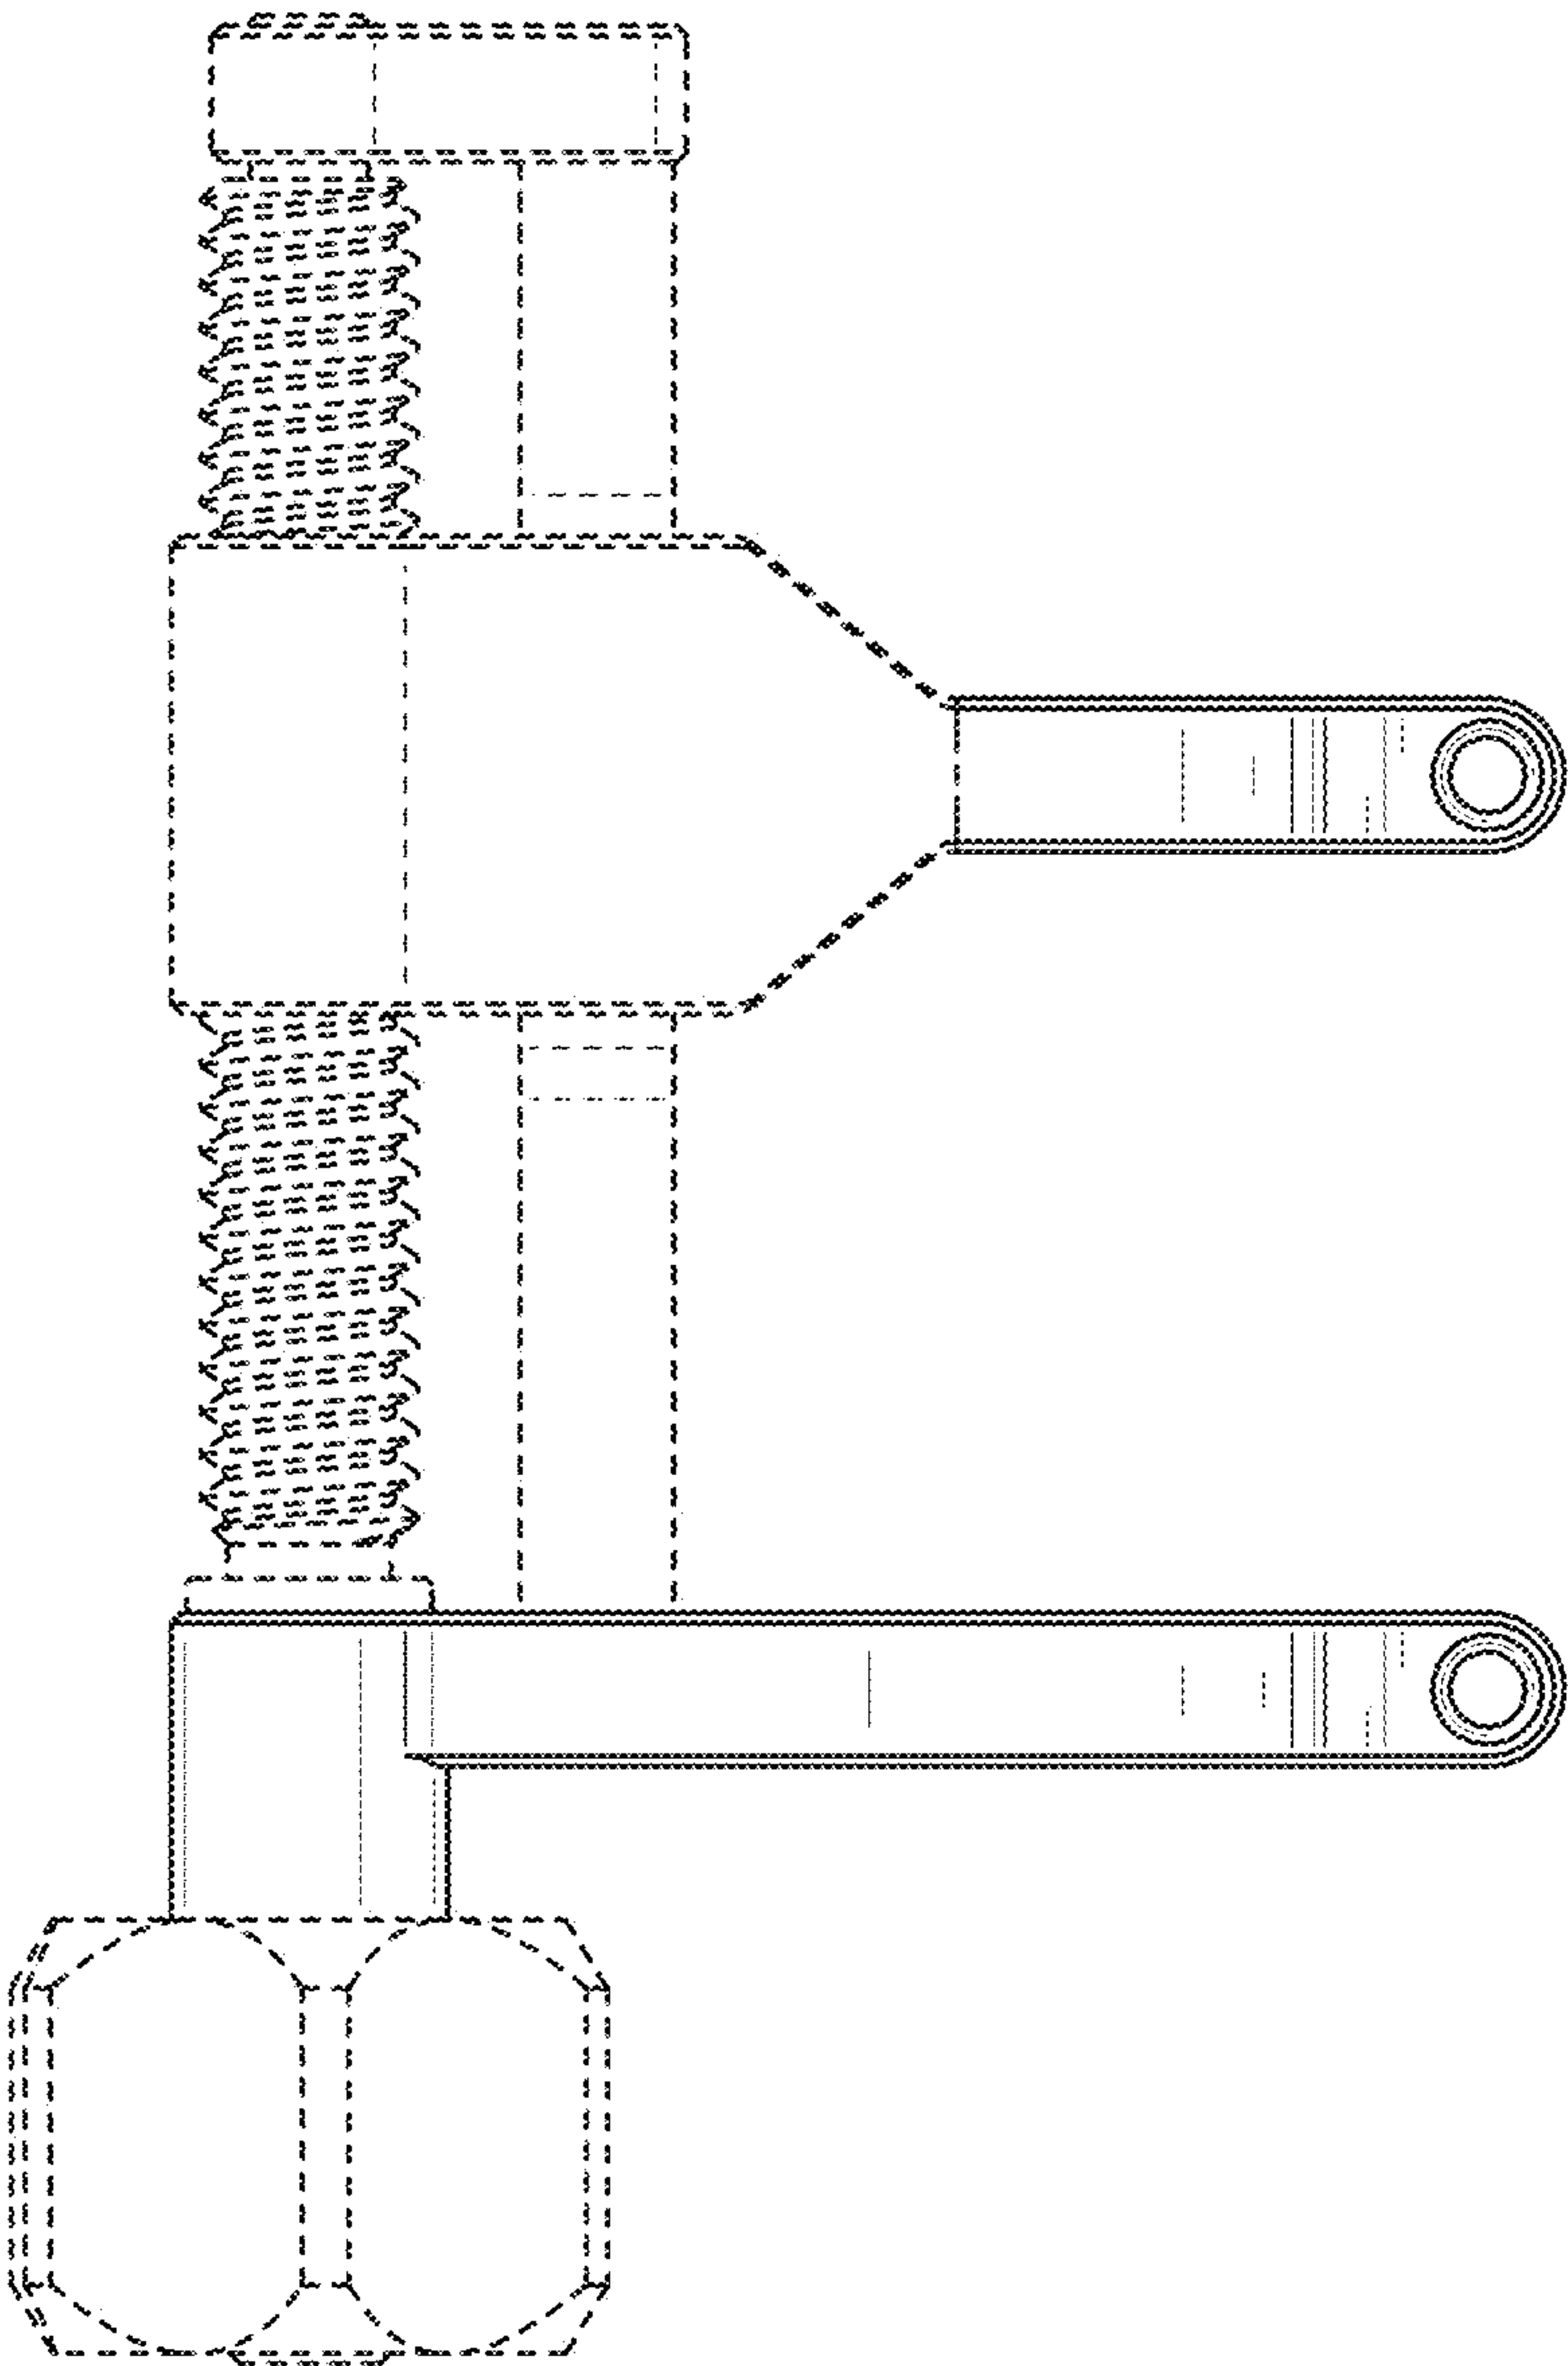


FIG. 6

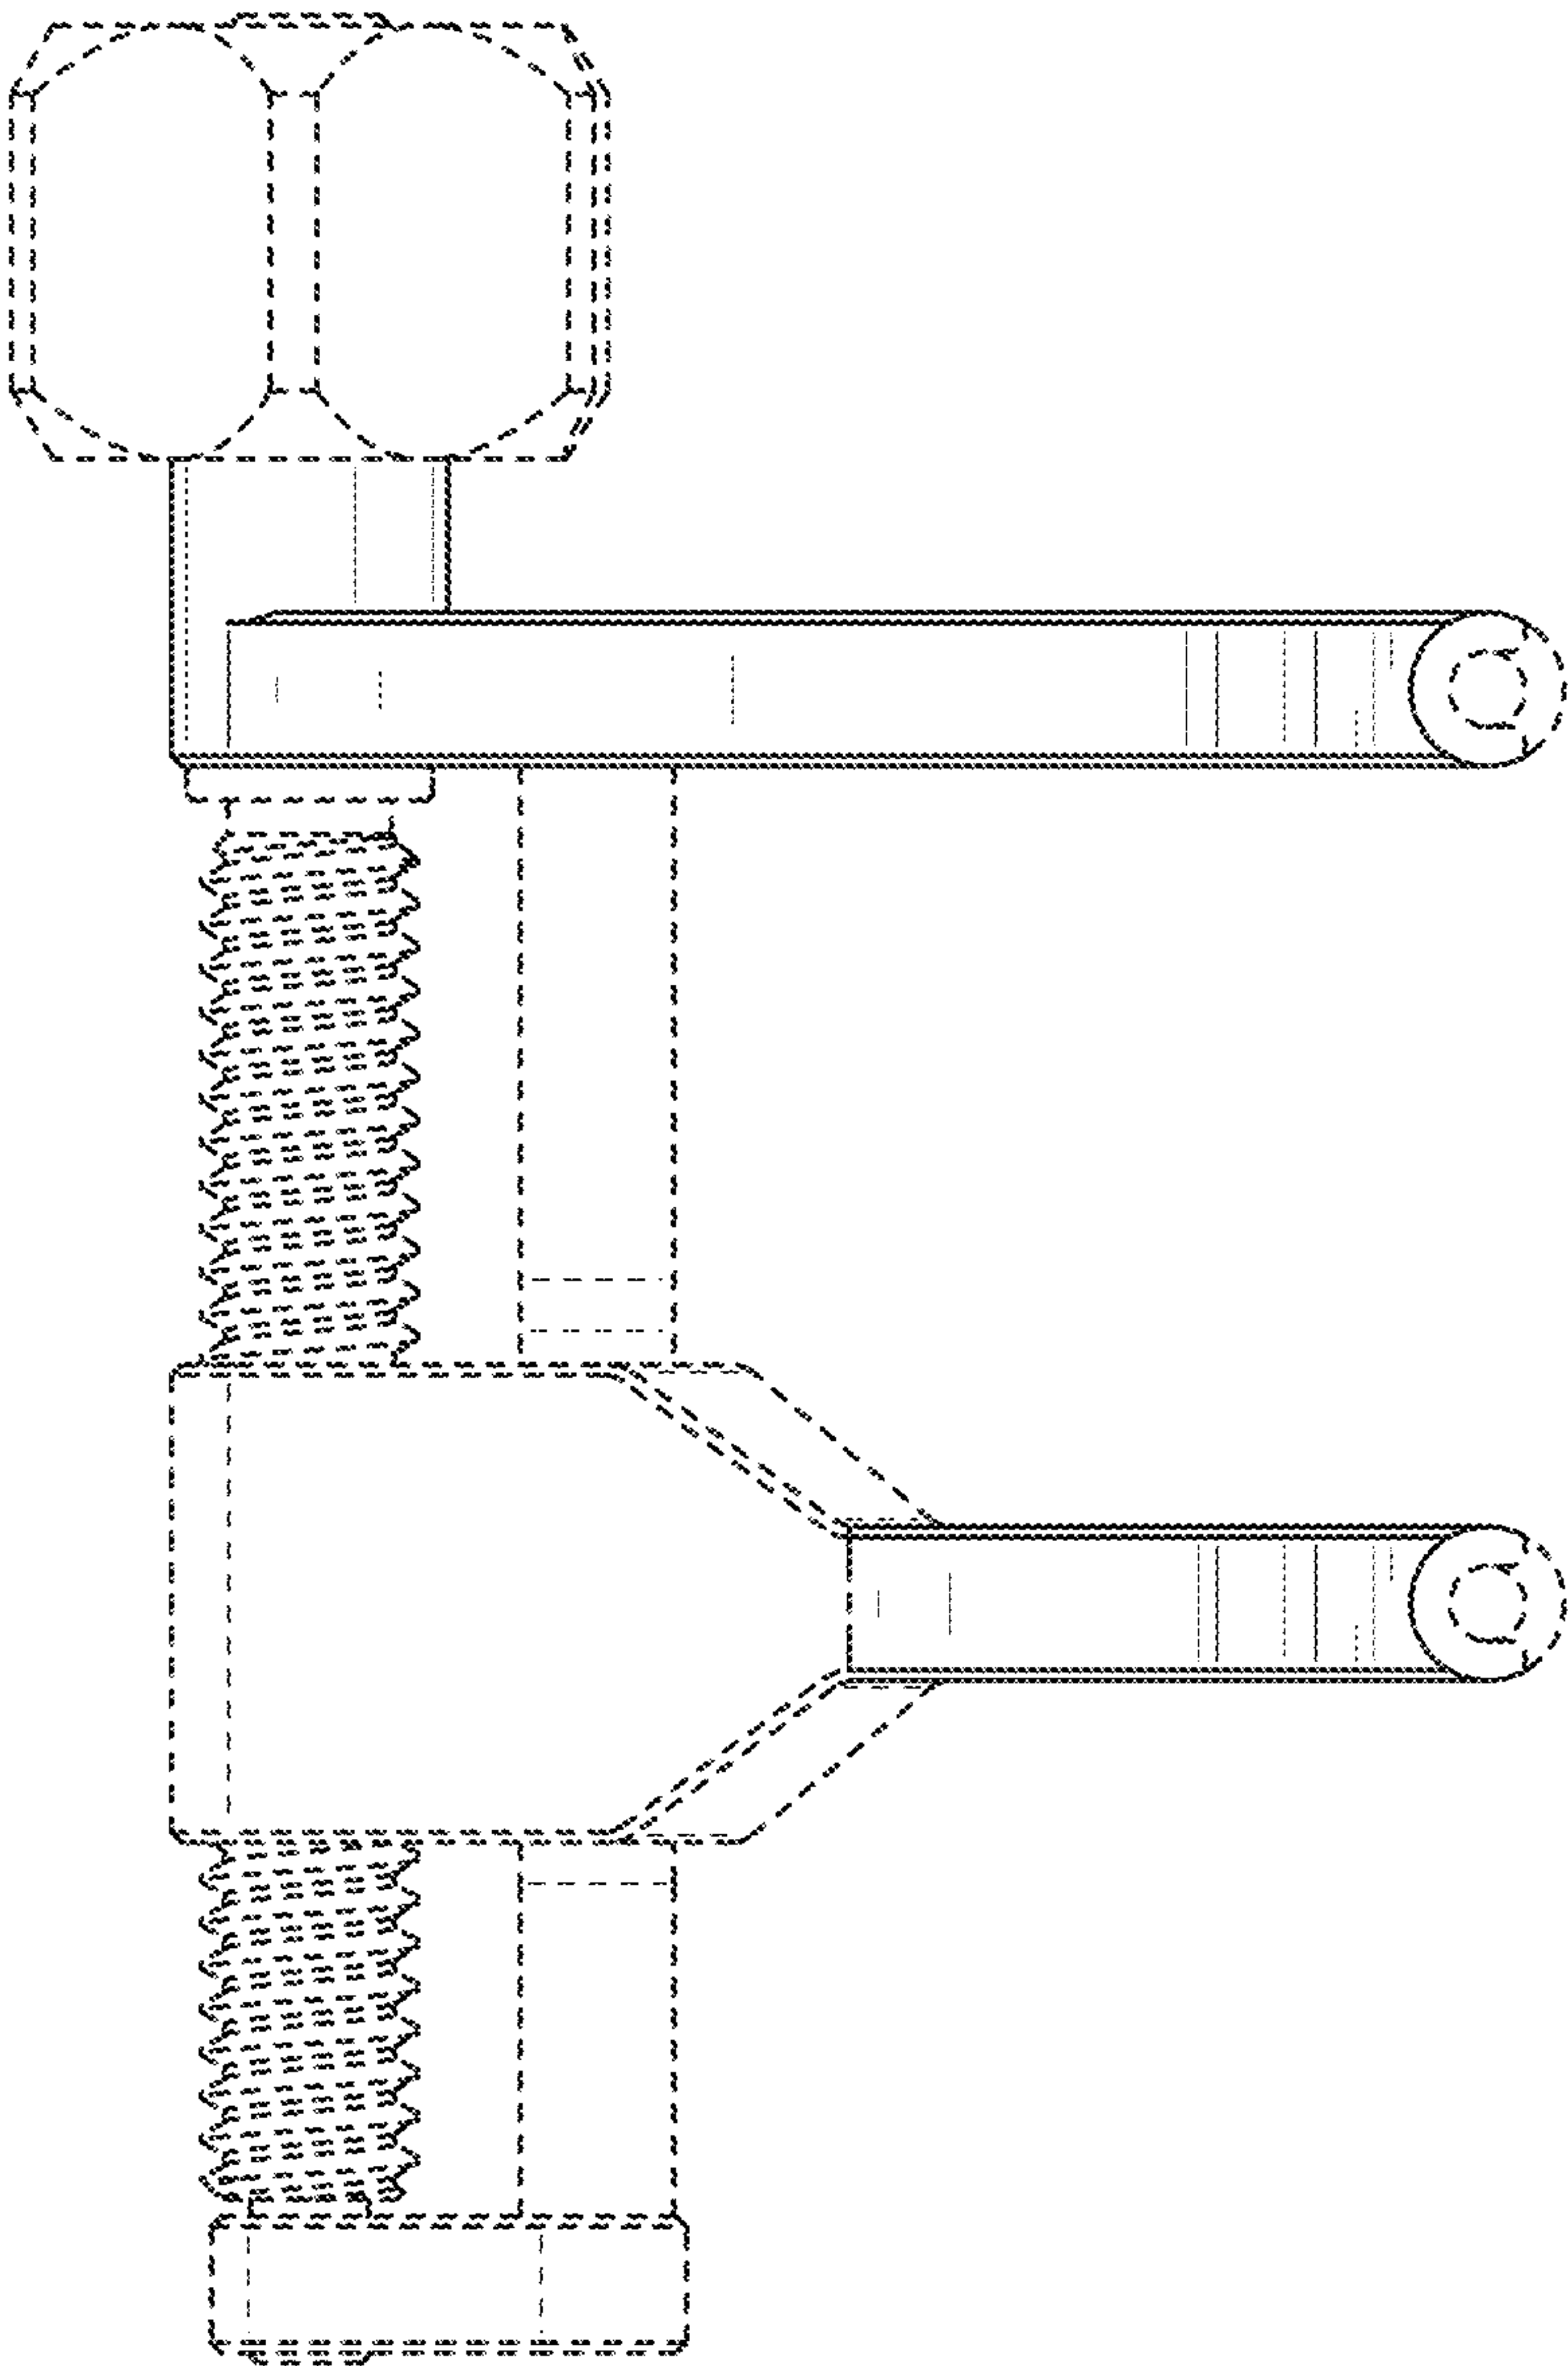


FIG. 7