



US0D1014774S

(12)

United States Design Patent

Wang et al.

(10)

Patent No.:

US D1,014,774 S

(45)

Date of Patent:

** Feb. 13, 2024

(54) STERILIZATION DEVICE

(71) Applicant: Delta Electronics, Inc., Taoyuan (TW)

(72) Inventors: Chih-Hsien Wang, Taoyuan (TW);
Shih-Chieh Chang, Taoyuan (TW);
Yan-Jun Wang, Taoyuan (TW);
Peng-Hui Wang, Taoyuan (TW);
Ming-Chieh Cheng, Taoyuan (TW);
Chuan-Hsi Chang, Taoyuan (TW)

(73) Assignee: DELTA ELECTRONICS, INC.,
Taoyuan (TW)

(**) Term: 15 Years

(21) Appl. No.: 29/828,164

(22) Filed: Feb. 24, 2022

(30) Foreign Application Priority Data

Feb. 21, 2022 (JP) 2022-003236 D

(51) LOC (14) Cl. 24-02

(52) U.S. Cl.

USPC D24/217

(58) Field of Classification Search

USPC D24/107, 177, 209, 210, 216, 217, 218,
D24/231, 232, 224, 227, 229; D23/217,
D23/218, 223, 355, 366; D32/1;
D26/37; D28/9, 73, 99

CPC ... A61L 2/025; A61L 2/07; A61L 2/10; A61L
2/24; A61L 2/26; A61L 2202/10; A61L
2202/11; A61L 2202/14; A61L 2202/23;
A61L 2202/122

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D359,546 S * 6/1995 Savage D23/207

D405,191 S * 2/1999 Matsunaga D24/217

D456,524 S * 4/2002 Hehenberger D24/217

D616,563 S * 5/2010 Huck D24/217

D845,488 S * 4/2019 Cahen D24/177

D938,063 S * 12/2021 Williamson D24/217

(Continued)

FOREIGN PATENT DOCUMENTS

CN 306132251 S 10/2020

CN 307813034 * 1/2023

(Continued)

OTHER PUBLICATIONS

“Baimnocm: Germicidal UVC Lamp.” Found online at amazon.
com. Aug. 7, 2023. Reference dated Jun. 27, 2022. Retrieved from
<https://www.amazon.com/dp/B0B56HW4XS/>.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton
Assistant Examiner — Elizabeth S Struble
(74) Attorney, Agent, or Firm — KIRTON McCONKIE;
Evan R. Witt

(57)


CLAIM

The ornamental design for a sterilization device, as shown
and described.

DESCRIPTION

FIG. 1 is a top, front, left perspective view of a sterilization
device showing our new design;
FIG. 2 is a bottom, rear, right perspective view thereof;
FIG. 3 is a front elevation view thereof;
FIG. 4 is a rear elevation view thereof;
FIG. 5 is a left side elevation view thereof;
FIG. 6 is a right side elevation view thereof;
FIG. 7 is a top plan view thereof; and,
FIG. 8 is a bottom plan view thereof.
The broken lines in the drawings depict portions of the
sterilization device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

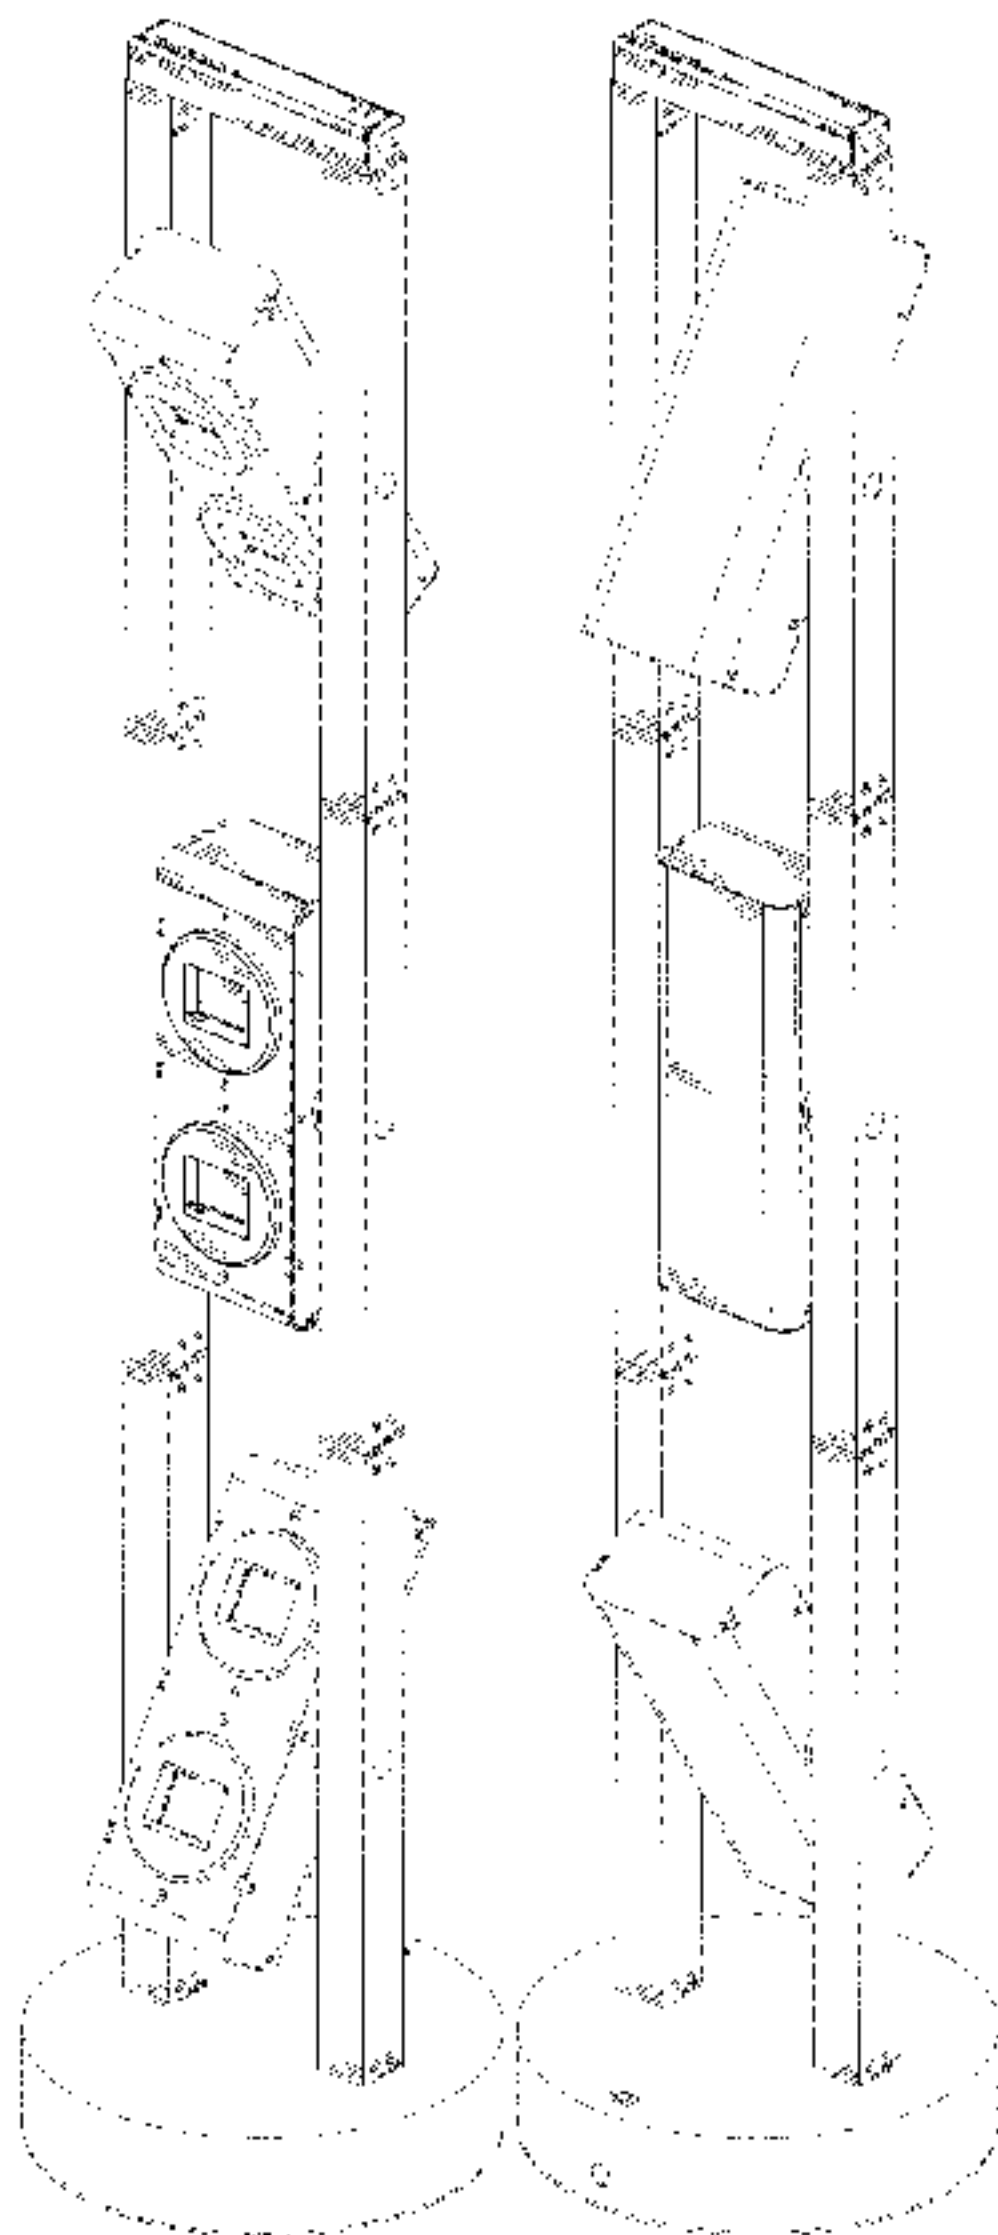

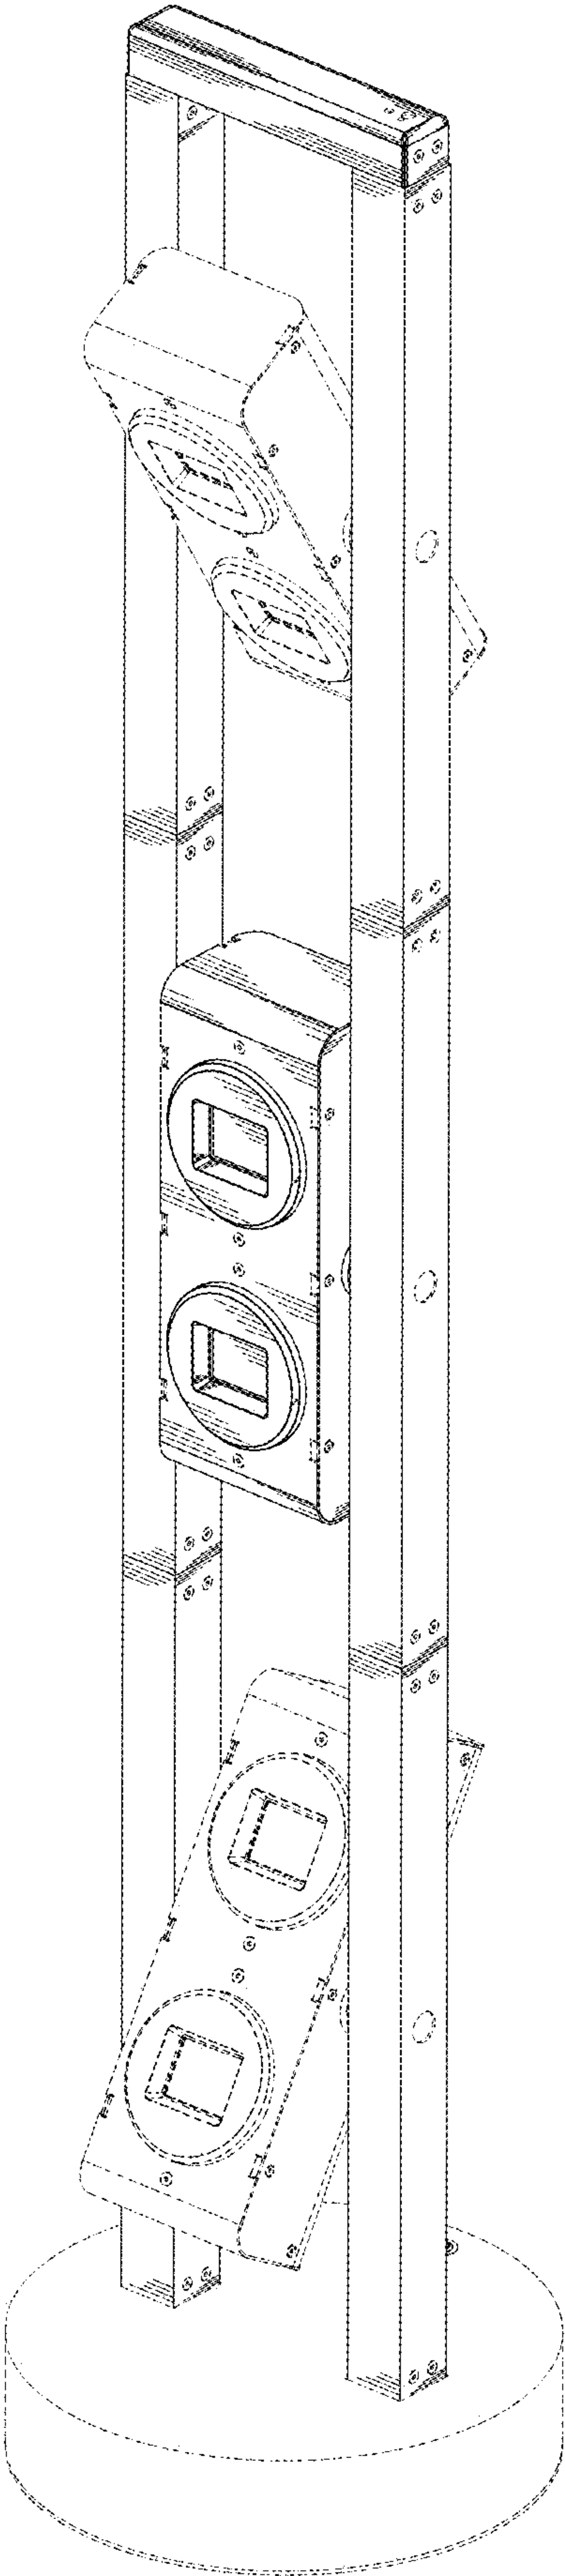


FIG. 1

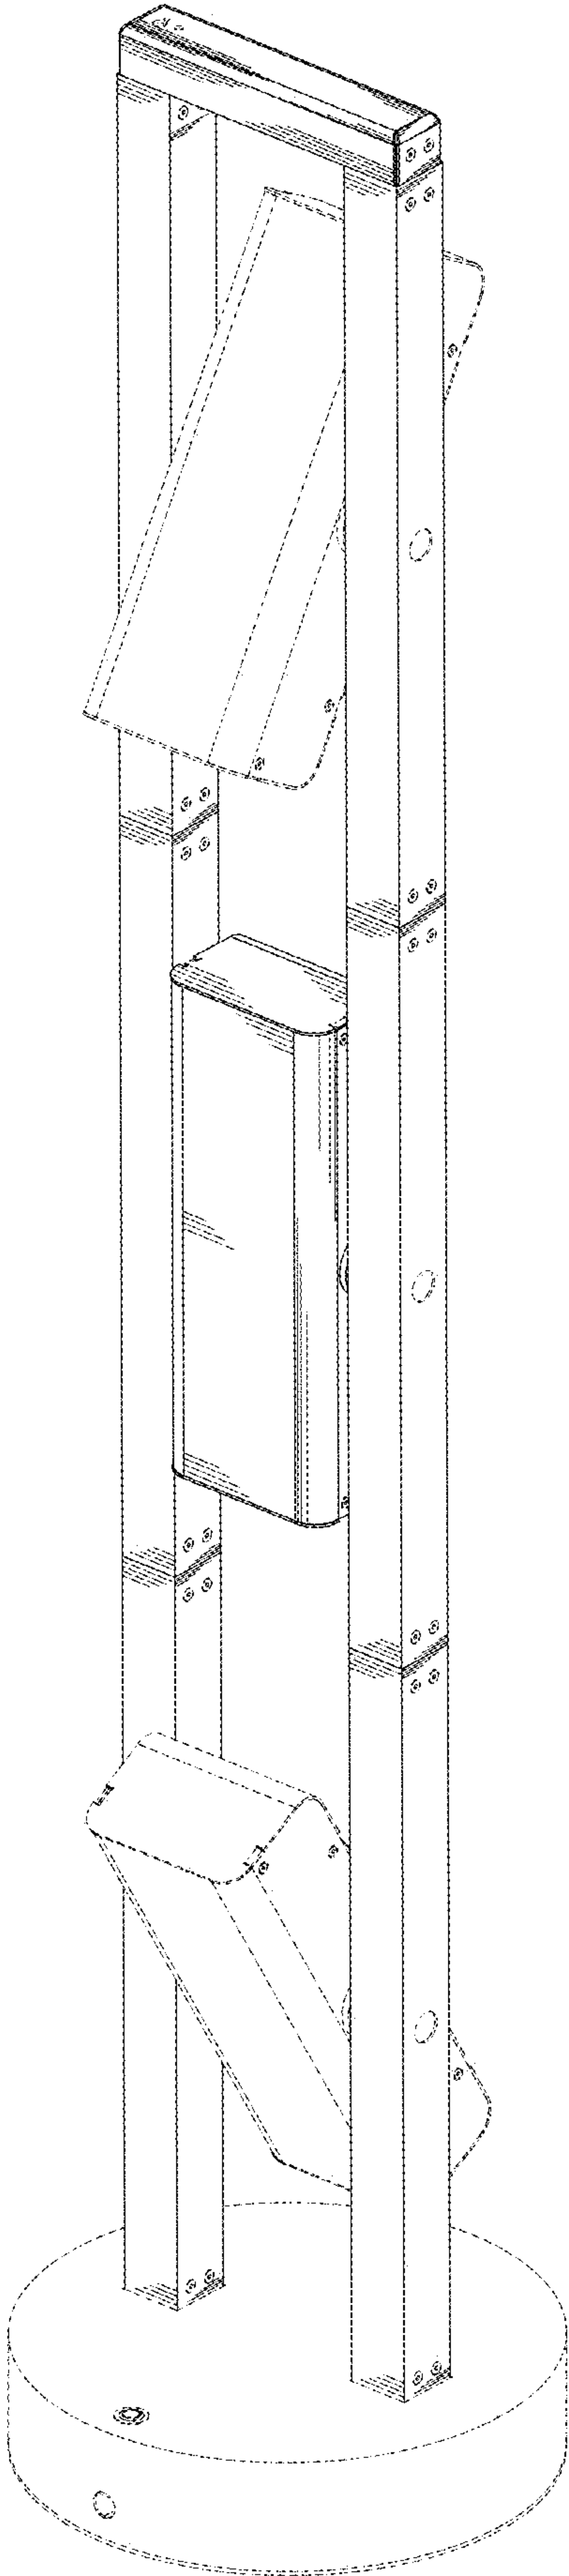


FIG. 2

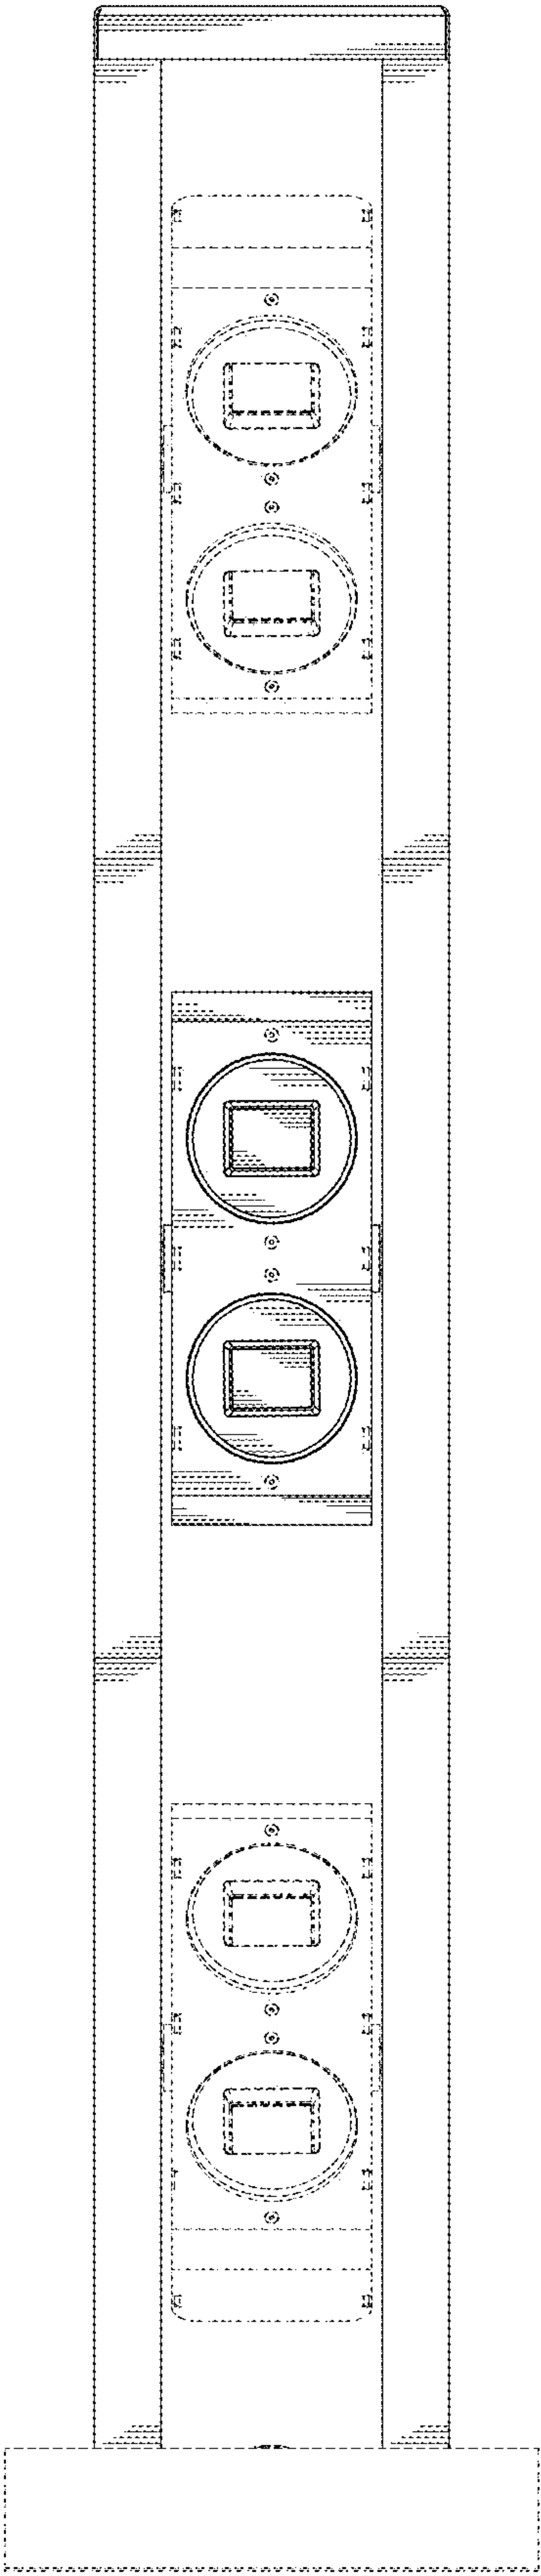


FIG. 3

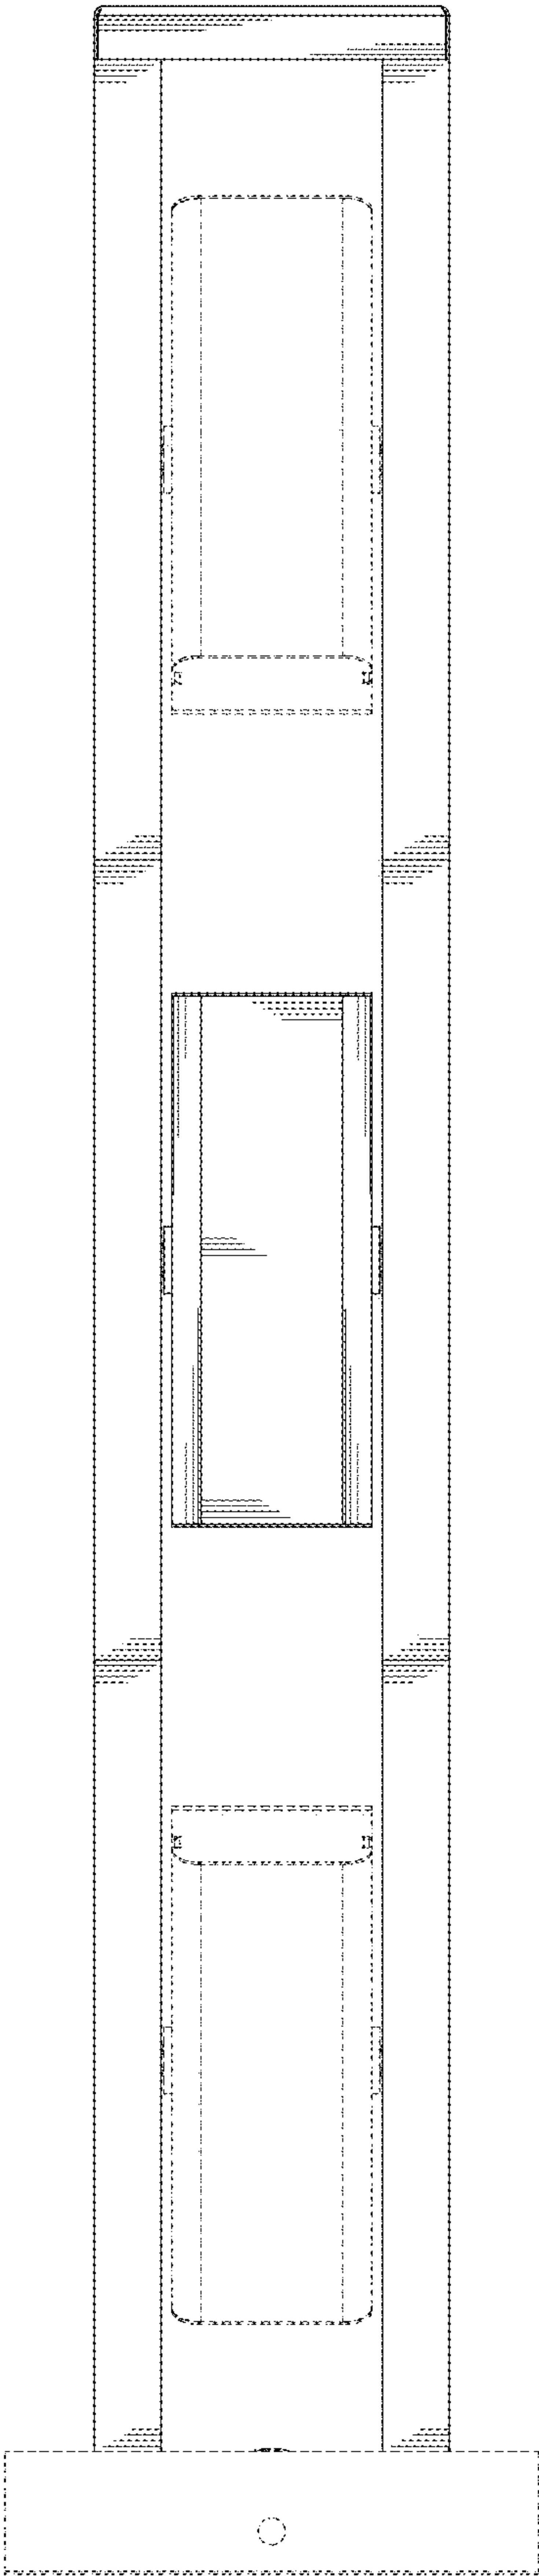


FIG. 4

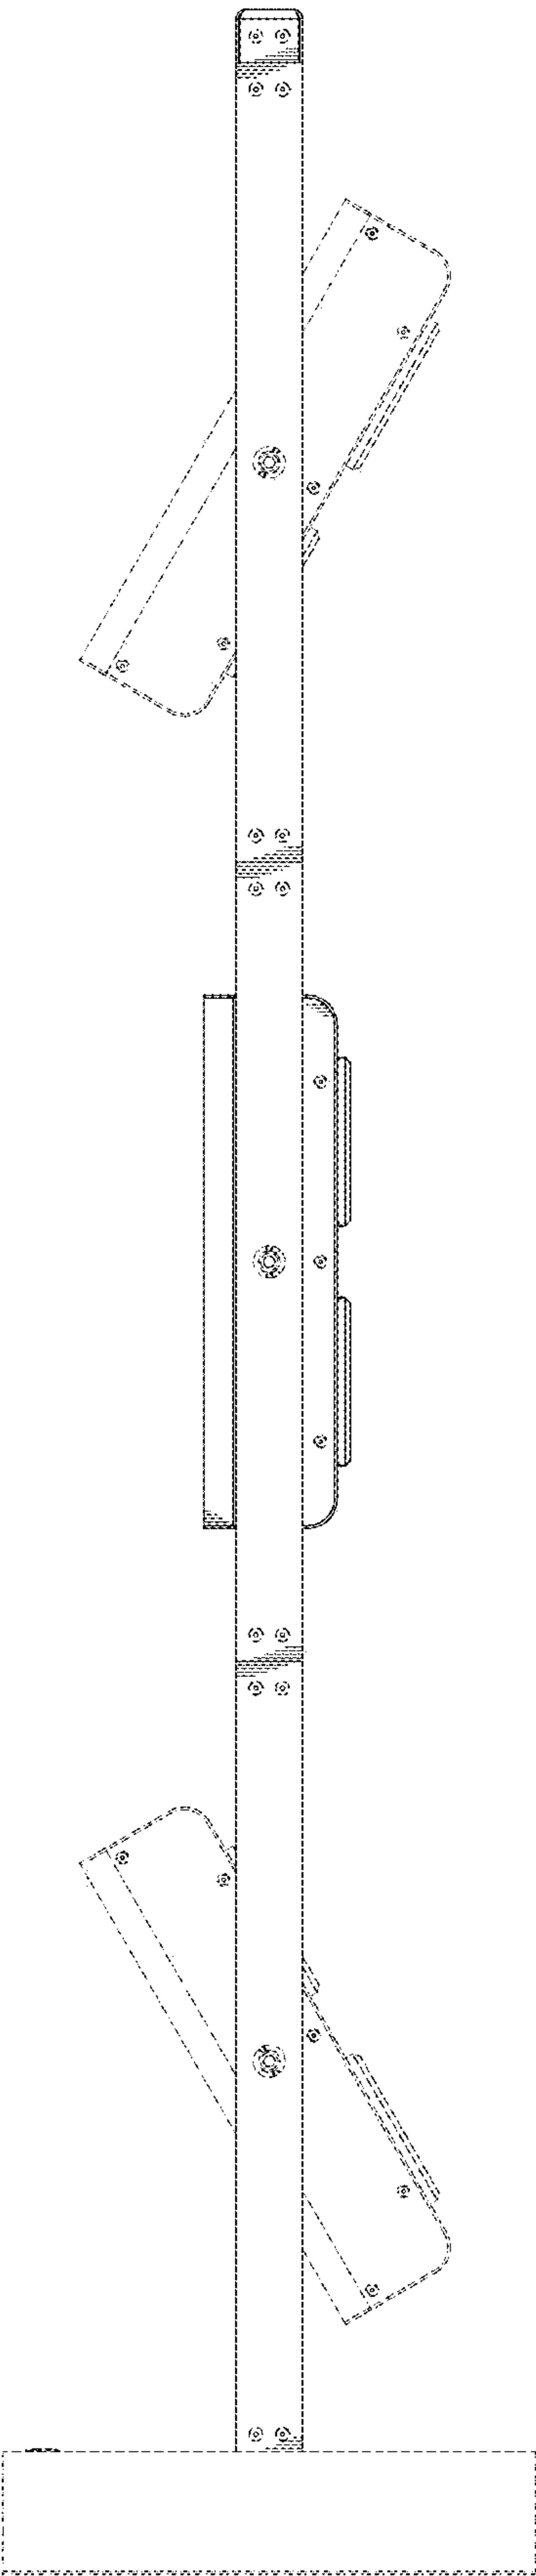


FIG. 5

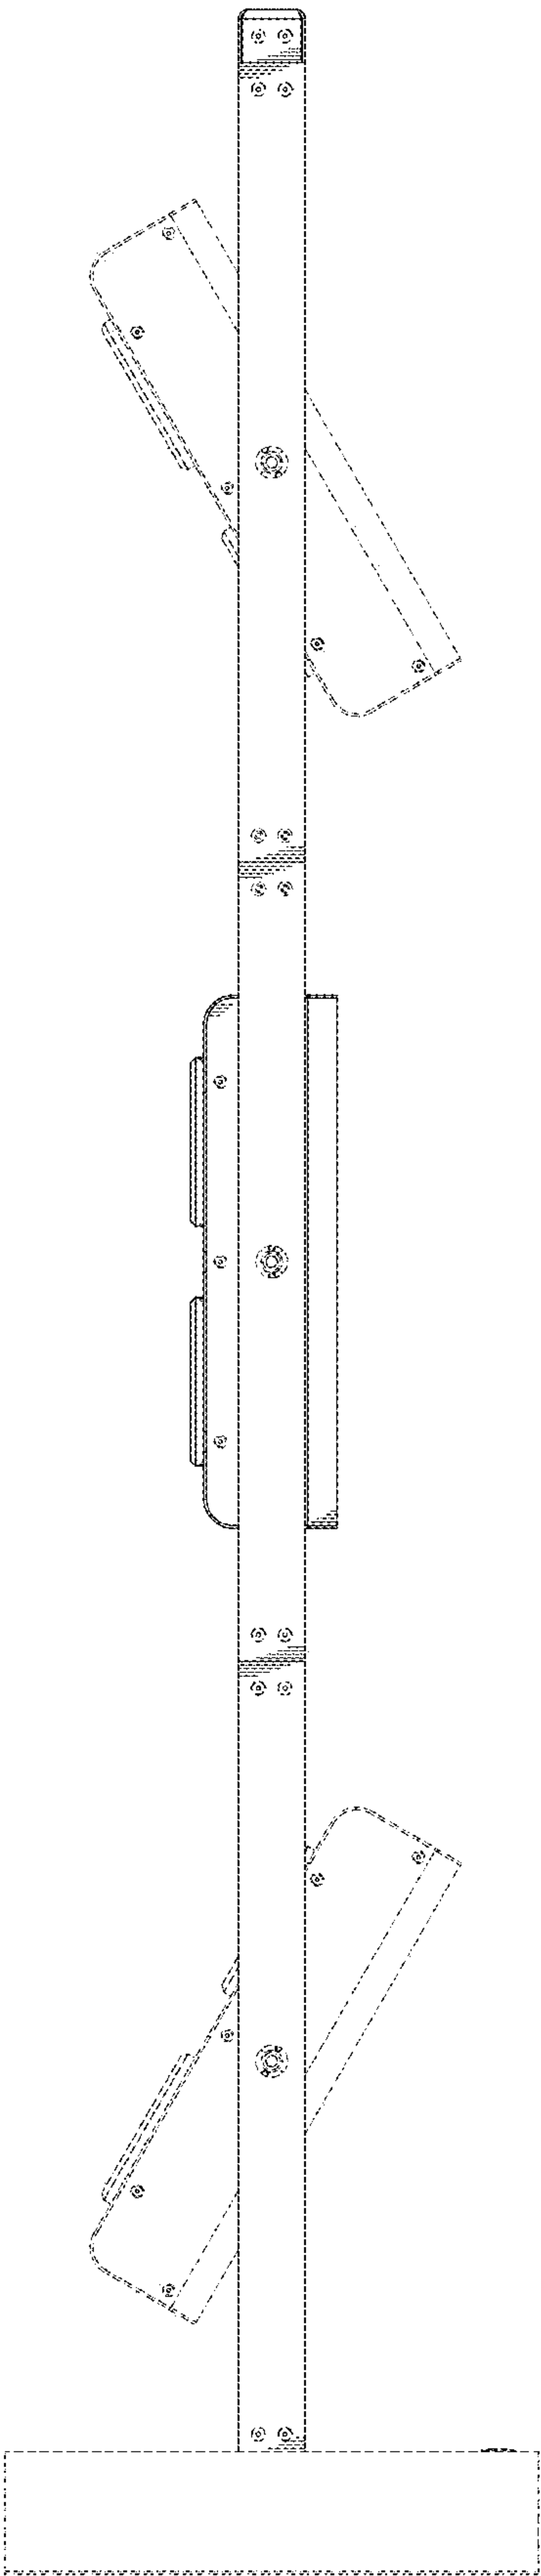


FIG. 6

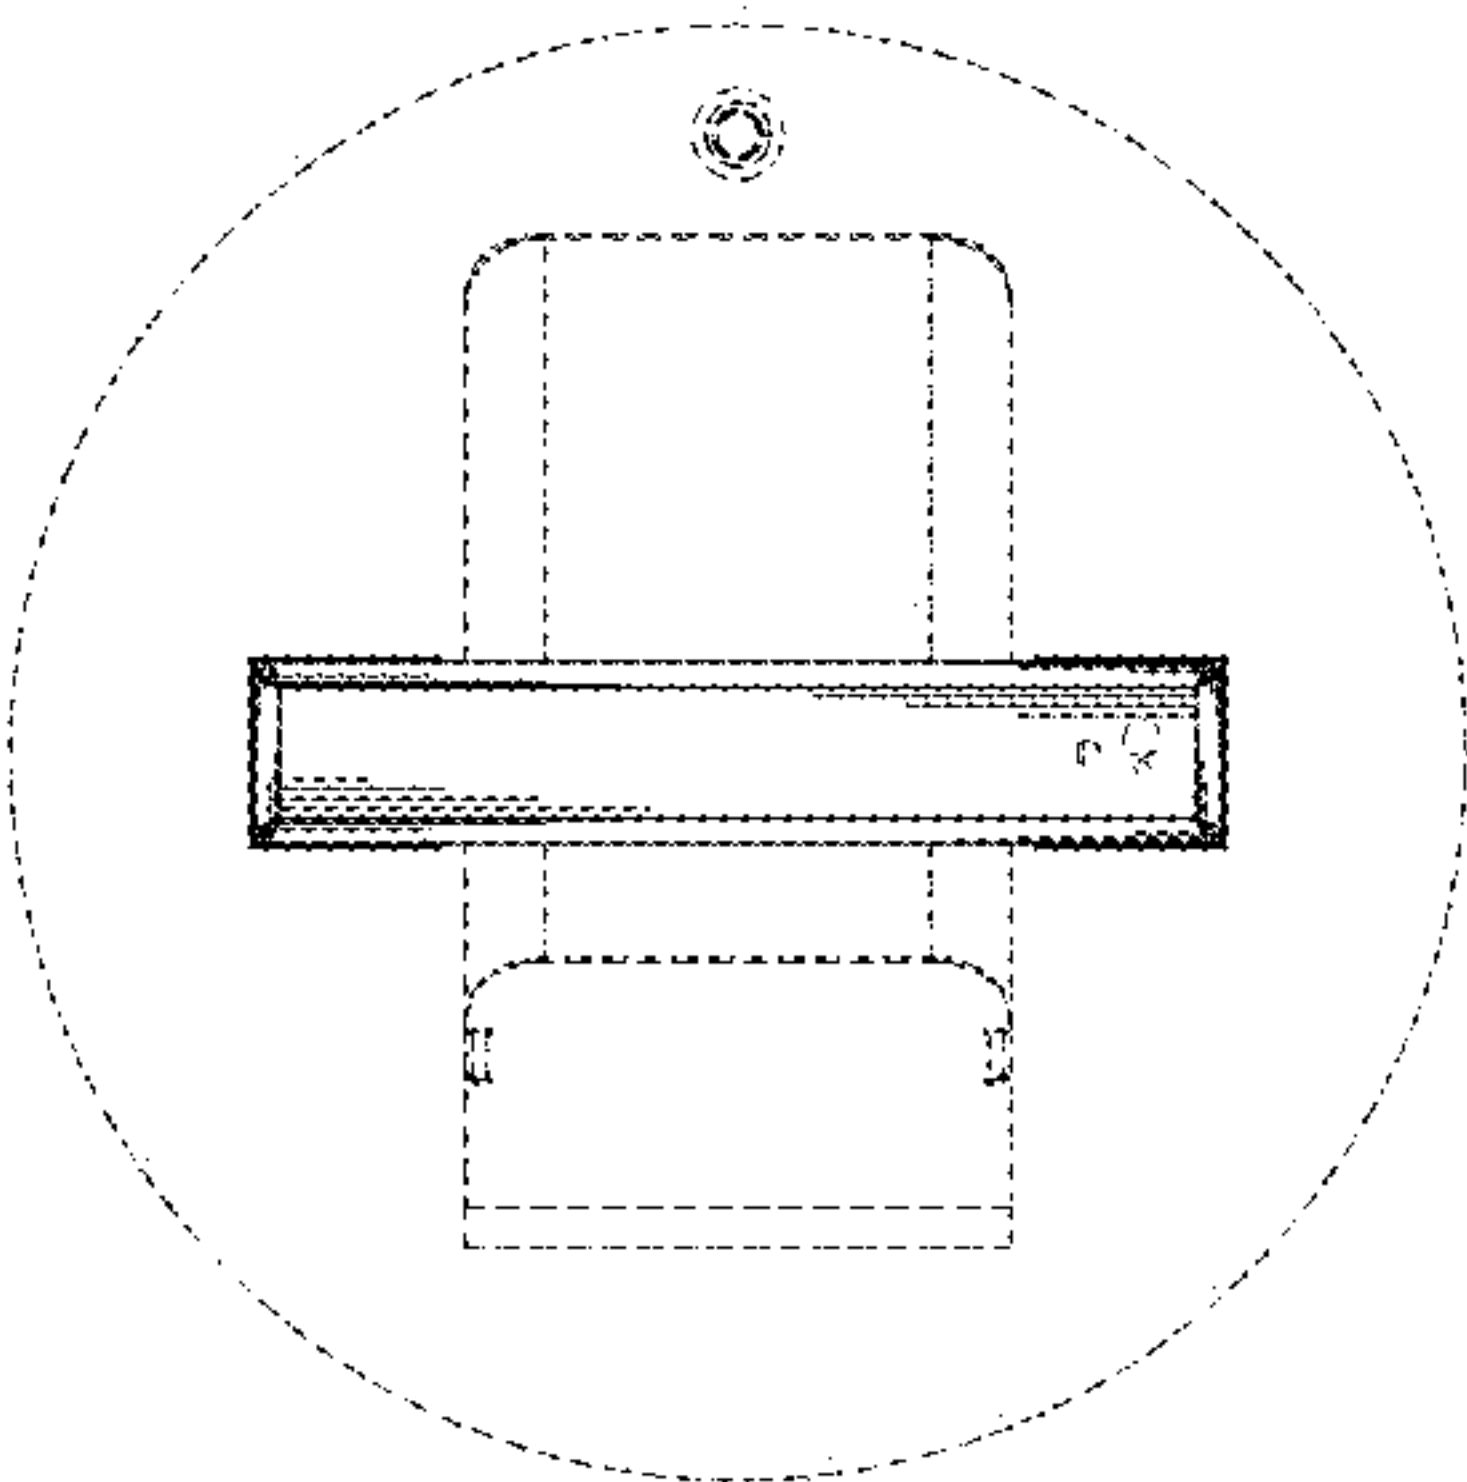


FIG. 7

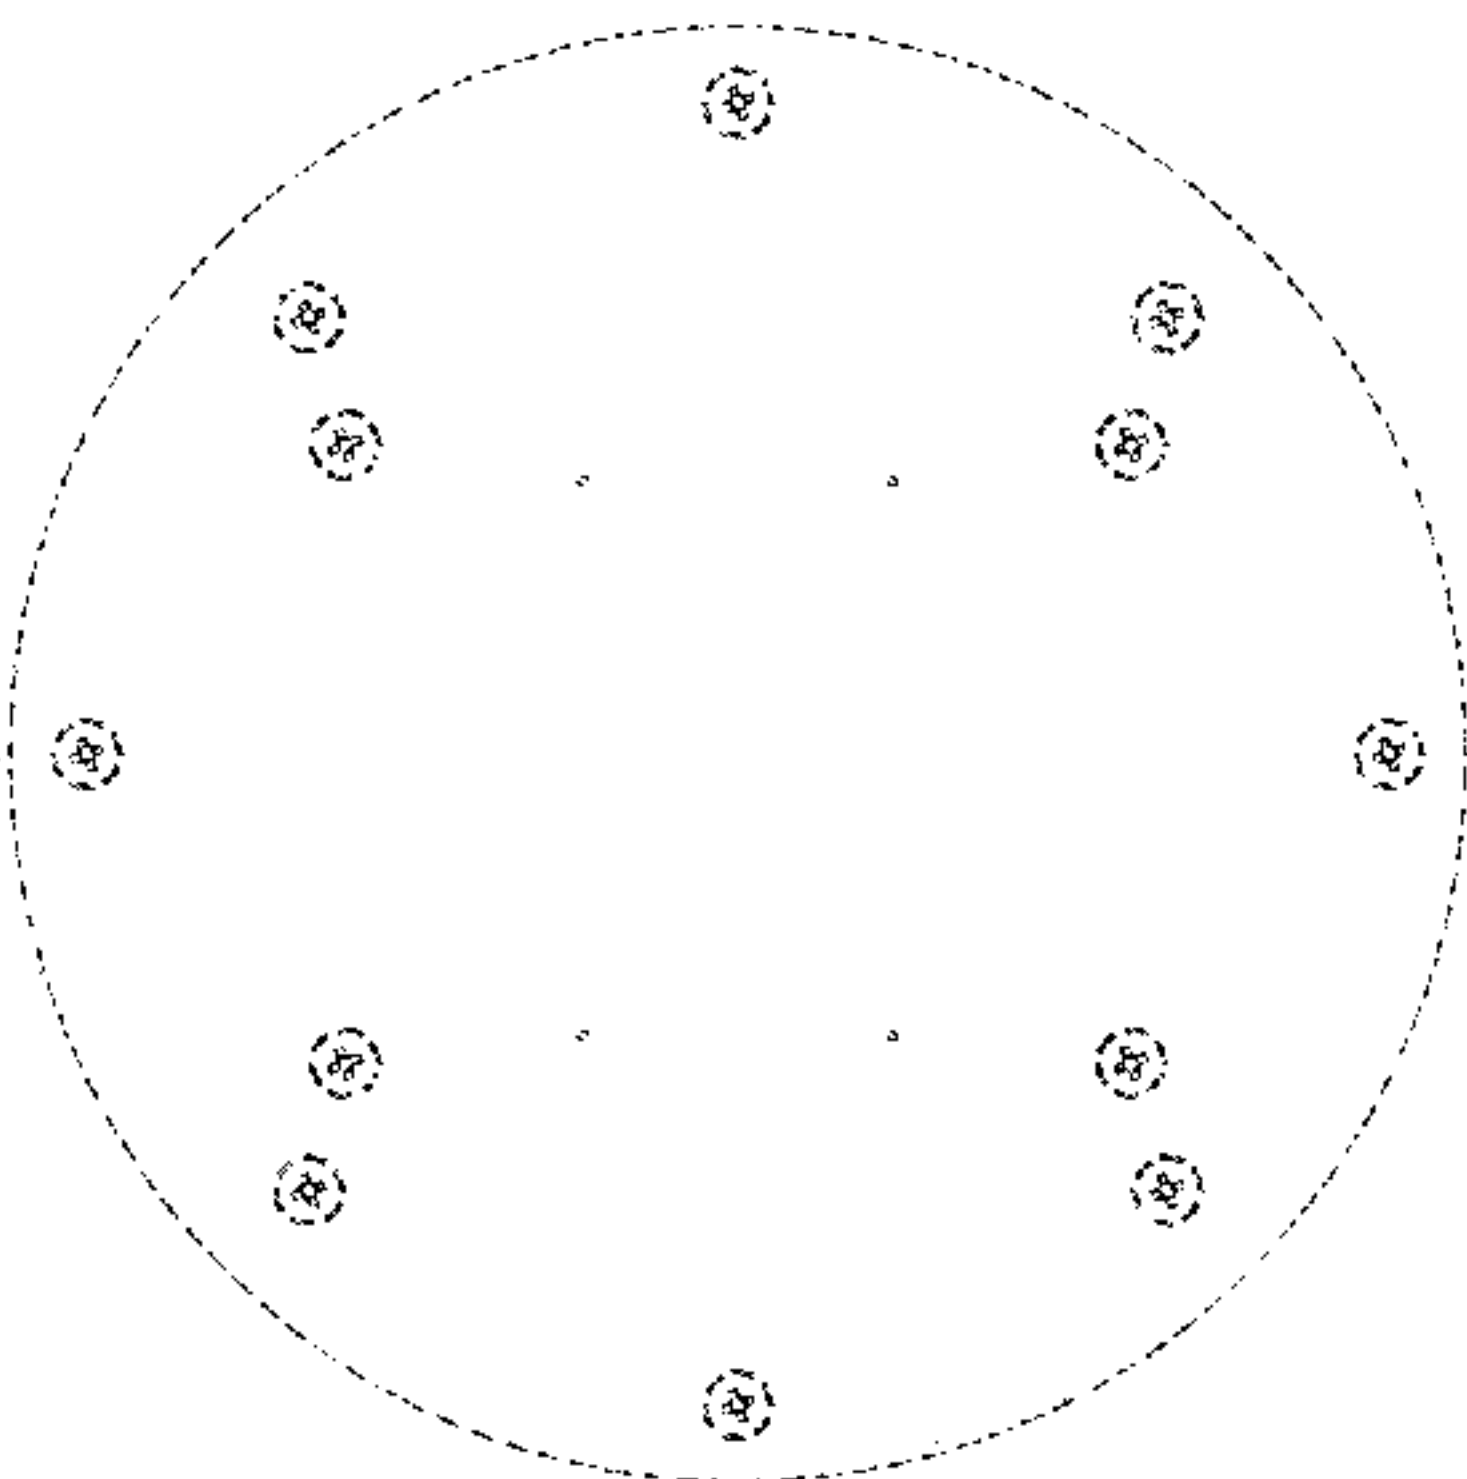


FIG. 8