



US0D1015535S

(12)

United States Design Patent

Matthison-Hansen et al.

(10) Patent No.: US D1,015,535 S

(45) Date of Patent: ** Feb. 20, 2024

(54) ENDOSCOPE HANDLE

(71) Applicant: AMBU A/S, Ballerup (DK)

(72) Inventors: Kaspar Mat Matthison-Hansen, Helsingør (DK); Tue Kjærgaard Toft, Kongens Lyngby (DK)

(73) Assignee: AMBU A/S, Ballerup (DK)

(**) Term: 15 Years

(21) Appl. No.: 29/790,573

(22) Filed: Dec. 3, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. D24/138

(58) Field of Classification Search

USPC D24/137, 138, 127, 130, 133, 134, 146, D24/147, 160, 107, 186

CPC A61B 1/00066; A61B 1/0052; A61B 1/2676; A61B 17/320016; A61B 1/00121; A61B 1/00124; A61B 1/00002; A61B 1/00018; A61B 1/00094; A61B 1/0661;

(Continued)

(56) References Cited

U.S. PATENT DOCUMENTS

D466,388 S * 12/2002 Chemtob D8/107

D481,124 S * 10/2003 Hayamizu D24/138

D498,846 S * 11/2004 Hayamizu D24/138

(Continued)

OTHER PUBLICATIONS

Medical Equipment Endoscopy System With LED Light Source, aliexpress.us, [online], [site visited date May 3, 2023], Available from the internet, URL: https://www.aliexpress.us/item/3256802814219970.html (Year: 2023).*

(Continued)

Primary Examiner — Samantha Q Lawrence

Assistant Examiner — Thanh Luu Wong

(74) Attorney, Agent, or Firm — Faegre Drinker Biddle & Reath LLP

(57) CLAIM

The ornamental design for an endoscope handle, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a first embodiment of an endoscope handle showing our new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof;

FIG. 6 is a top view thereof; and

FIG. 7 is a bottom view thereof.

FIG. 8 is a front perspective view of a second embodiment of an endoscope handle showing our new design;

FIG. 9 is a front view thereof;

FIG. 10 is a rear view thereof;

FIG. 11 is a left side view thereof;

FIG. 12 is a right side view thereof;

FIG. 13 is a top view thereof; and

FIG. 14 is a bottom view thereof.

FIG. 15 is a front perspective view of a third embodiment of an endoscope handle showing our new design;

FIG. 16 is a front view thereof;

FIG. 17 is a rear view thereof;

FIG. 18 is a left side view thereof;


FIG. 19 is a right side view thereof;

FIG. 20 is a top view thereof; and,

FIG. 21 is a bottom view thereof.

Long-short broken lines illustrate boundaries that form no part of the claimed design. Evenly-sized broken lines illustrate portions of the endoscope handle that form no part of the claimed design.

1 Claim, 15 Drawing Sheets

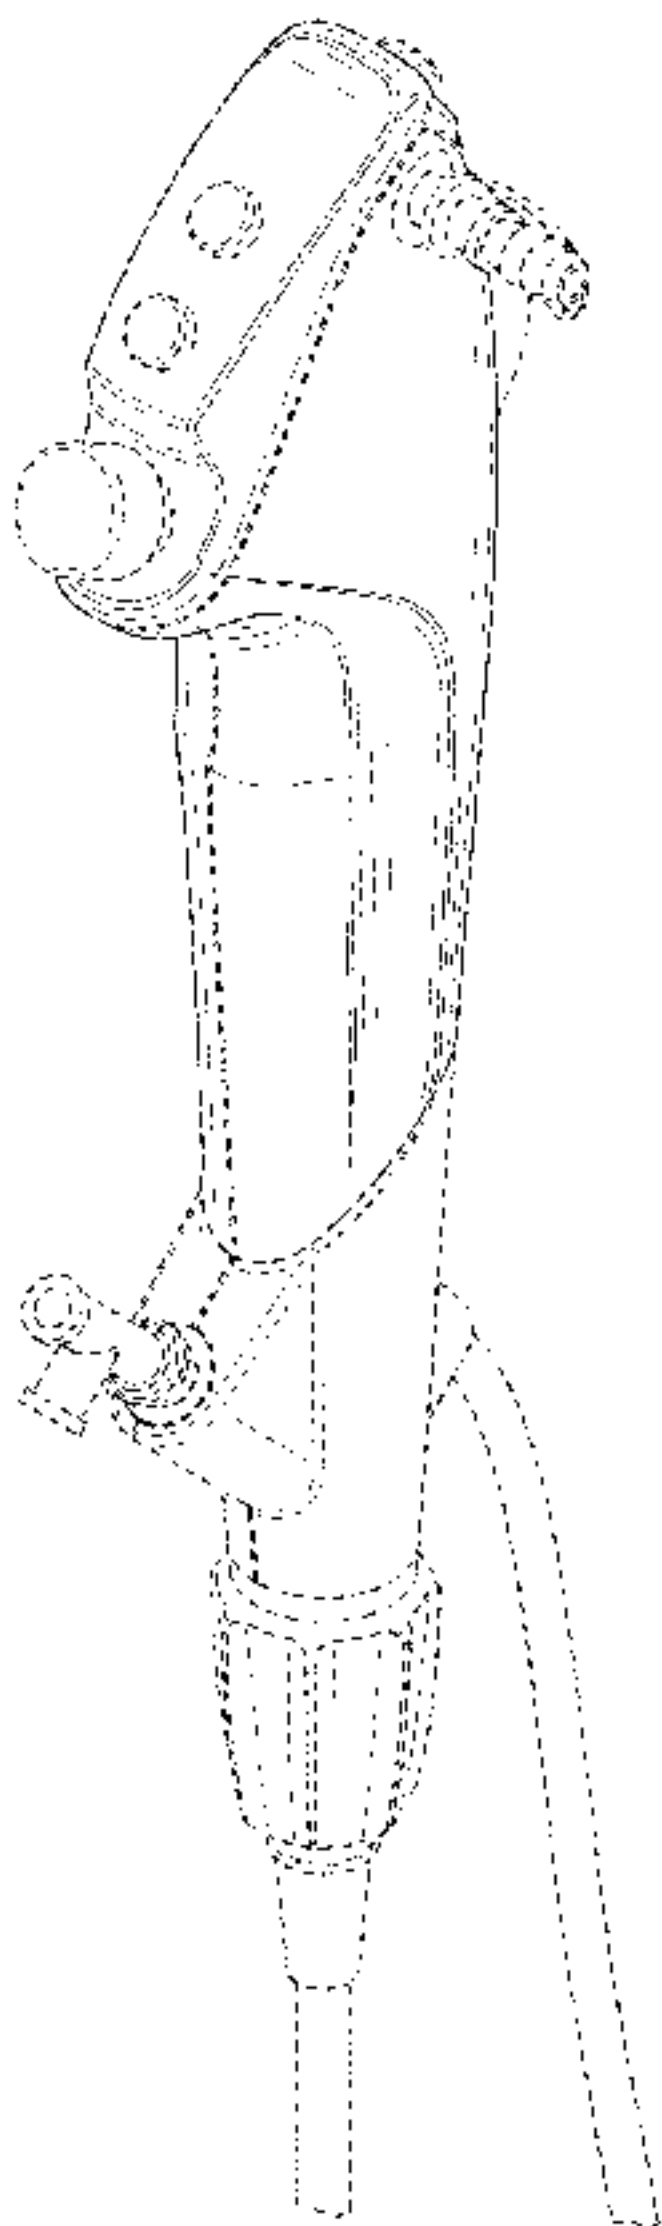

(58) Field of Classification Search

CPC A61B 1/00064; A61B 1/00112; A61B 17/3478; A61M 25/0136
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D660,430	S	*	5/2012	Horning		D24/146
D669,175	S	*	10/2012	Makowski		D24/138
9,179,831	B2	*	11/2015	McGrail		G02B 23/2423
D753,298	S	*	4/2016	Hayamizu		D24/138
D760,895	S	*	7/2016	McMahon		D24/137
D777,915	S	*	1/2017	Tanaka		D24/138
D782,672	S	*	3/2017	Tanaka		D24/138
10,779,710	B2	*	9/2020	Matthison-Hansen		A61B 1/018
D898,910	S	*	10/2020	Hansen		D24/137
D902,401	S	*	11/2020	Ohno		D24/138
D935,017	S	*	11/2021	Kawanishi		D24/138
D936,221	S	*	11/2021	Jensen		D24/138
D937,412	S	*	11/2021	Ubbesen		D24/129
11,202,554	B2	*	12/2021	Lund		A61B 1/00105
D940,863	S	*	1/2022	Kawanishi		D24/138
D945,612	S	*	3/2022	Lund		D24/138
D950,726	S	*	5/2022	Kang		D24/138
D956,972	S	*	7/2022	Costin		A61B 1/317
D958,344	S	*	7/2022	Ono		D24/138
D958,346	S	*	7/2022	Ono		D24/138
D958,347	S	*	7/2022	Ono		D24/138
D964,561	S	*	9/2022	Suzuki		D24/138
D970,004	S	*	11/2022	Ohno		D24/138
D970,005	S	*	11/2022	Ohno		D24/138
D970,006	S	*	11/2022	Ohno		D24/138
D974,555	S	*	1/2023	Suzuki		D24/138
D975,275	S	*	1/2023	Ueda		D24/138
2020/0229684	A1	*	7/2020	Lund		A61B 1/00066
2020/0323418	A1	*	10/2020	Narayana		A61B 1/00133
2021/0275001	A1	*	9/2021	Lund		A61B 1/00066
2023/0018783	A1	*	1/2023	Kawanishi		A61B 1/005

OTHER PUBLICATIONS

Judex Video Endoscopes, judexmedical.com, [online], [site visited date May 3, 2023], Available from the internet, URL: <http://www.judexmedical.com/video-endoscopes.html> (Year: 2023).*

EndoFresh Obtains FDA 510(k) Clearance. prnewswire.com, May 24, 2021 [retrieved on May 3, 2023]. Retrieved from the Internet: <URL: <https://www.prnewswire.com/news-releases/endofresh-obtains-fda-510k-clearance-for-its-groundbreaking-disposable-digestive-endoscopy-system-301297399.html>> (Year: 2021).*

Liang, Z., Zhou, G., Li, Y. et al. Evaluation of a new developed disposable and portable bronchoscopy system. BMC Pulm Med 22, 136 (2022). <https://doi.org/10.1186/s12890-022-01933-z>. Fig. 1, “YunSendo-R bronchoscope”. (Year: 2022).*

Vathin Single-Use Flexible Ureteroscope, futuremedglobal.com, [online], [site visited Aug. 4, 2023], Available from internet, URL: <https://futuremedglobal.com/products/single-use-digital-flexible-ureteroscope> (Year: 2023).*

Screen captures from YouTube video clip entitled “Pusen Fully Flexible Video Single Use Ureteroscope PU3022A”, uploaded on Apr. 19, 2017 by user “Zhuhai Pusen Medical Technology”. Retrieved from Internet <<https://www.youtube.com/watch?v=JuHUDzvrtDs>> (Year: 2017).*

LithoVue. Product Brochure [online]. Boston Scientific, Jul. 2016 [retrieved on Aug. 4, 2023]. Retrieved from the Internet: <<https://www.bostonscientific.com/content/dam/bostonscientific/uro-wh/portfolio-group/LithoVue/LithoVue%20Product%20Shots/SupportingMaterials/LithoVue-Brochure.pdf>> (Year: 2016).*

BD Aptra Single-Use Digital Flexible Ureteroscope, bd.com, [online], [site visited Aug. 4, 2023], Available from internet, URL: <https://www.bd.com/en-us/products-and-solutions/products/product-page.bdsd01#specifications> (Year: 2023).*

Duomed Single-use Bronchoscopes, duomed.com, [online], [site visited Aug. 4, 2023], Available from internet, URL: <https://www.duomed.com/en-BE/h-steriscope-single-use-bronchoscope> (Year: 2023).*

Exalt Model B, FDA clearance announcement dated Aug. 10, 2021.

* cited by examiner

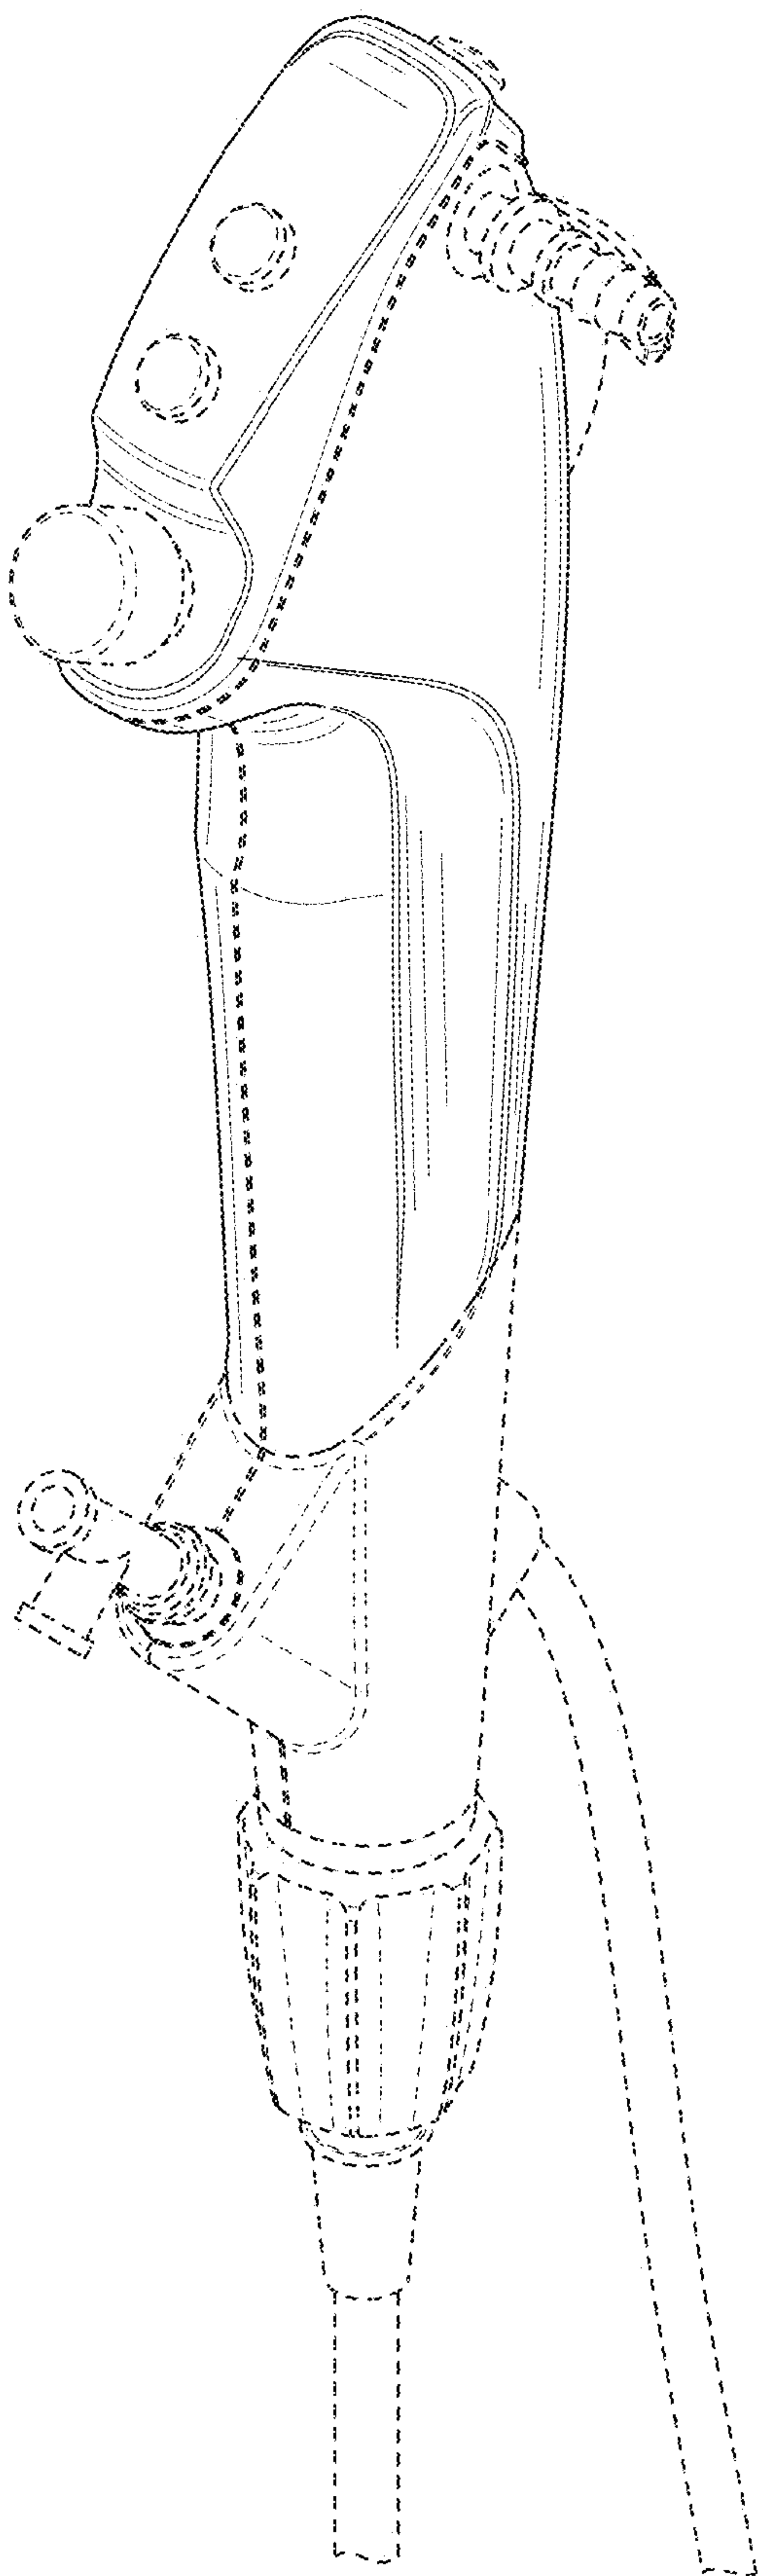


FIG. 1

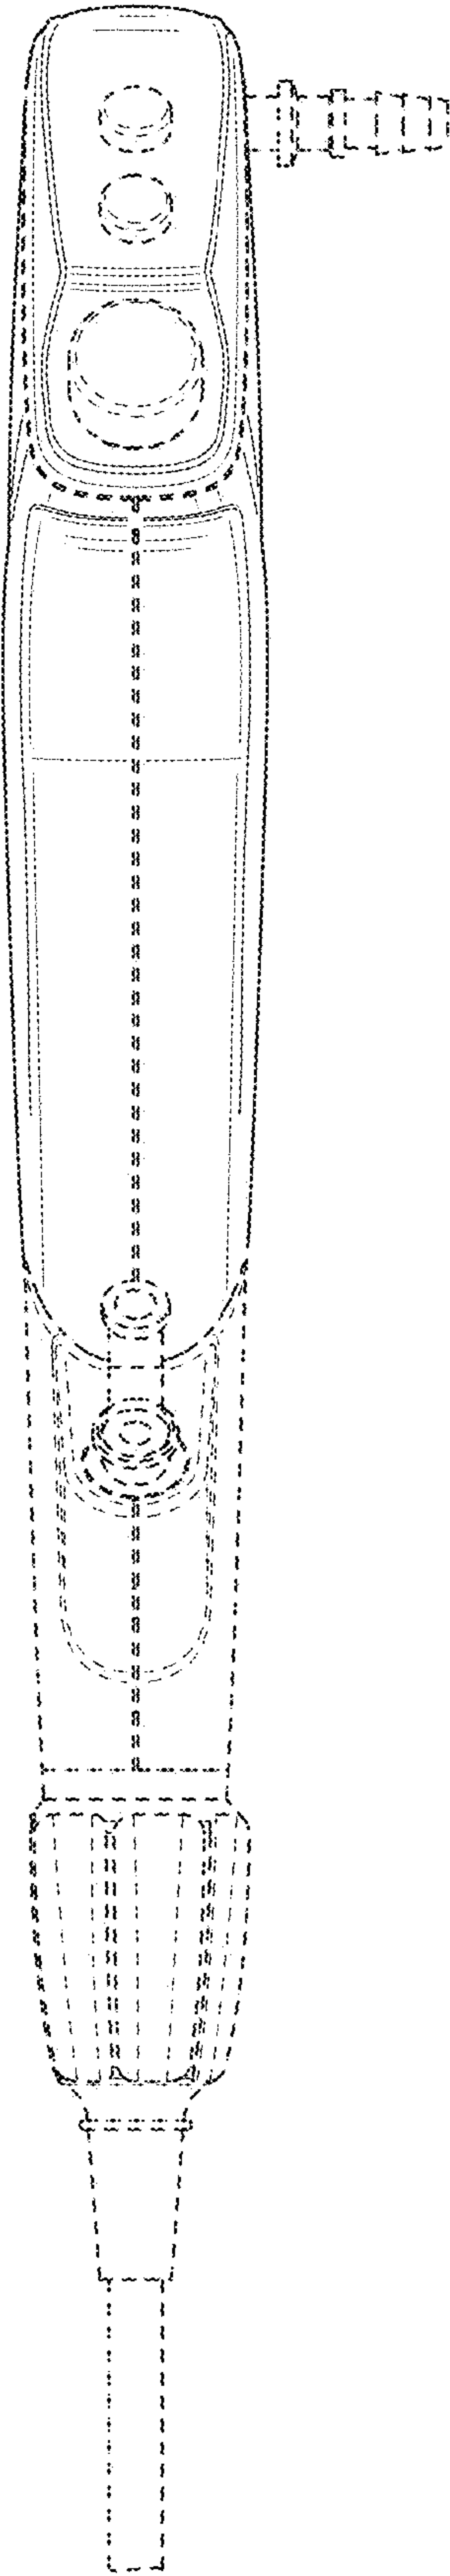


FIG. 2

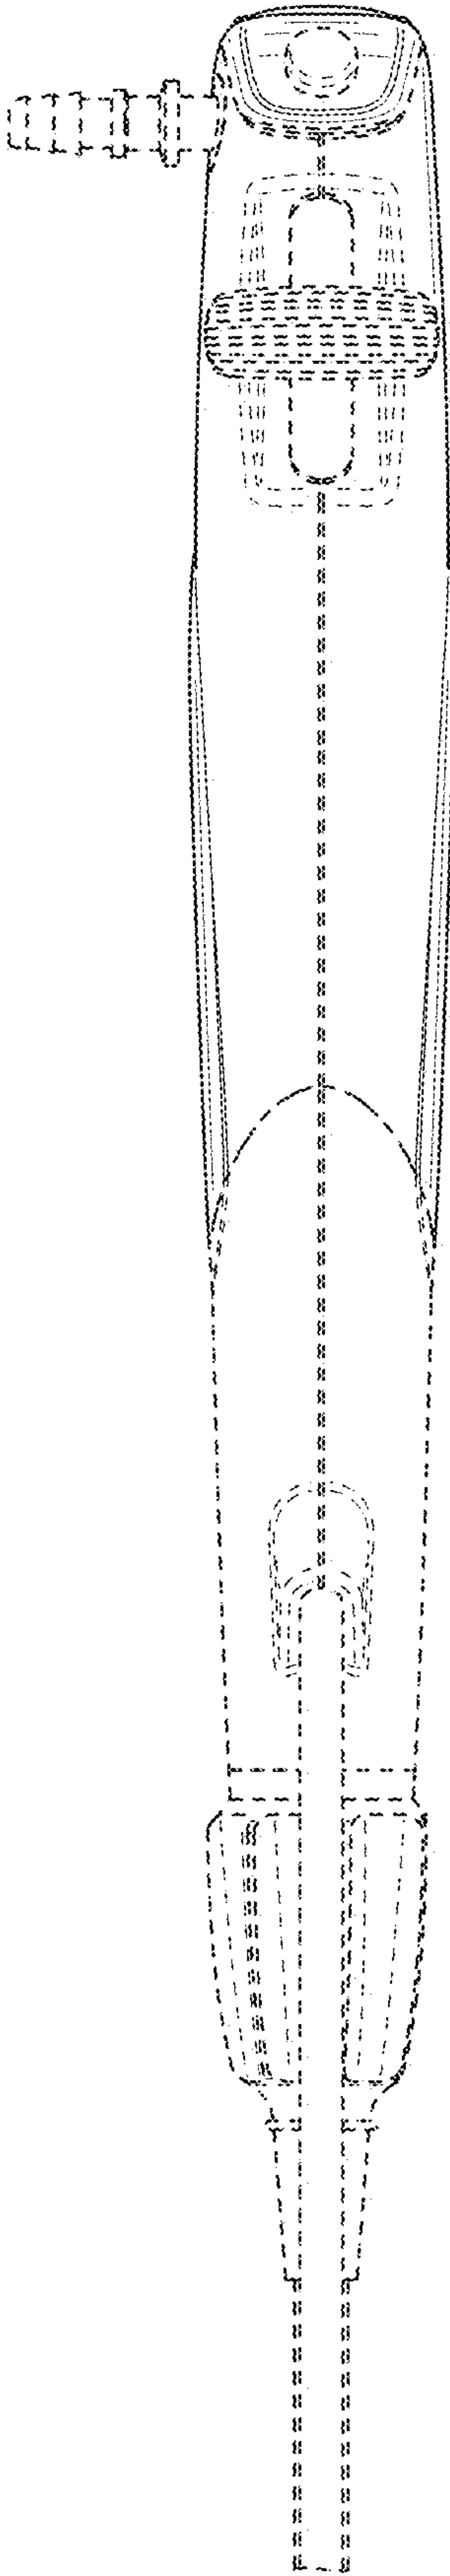


FIG. 3

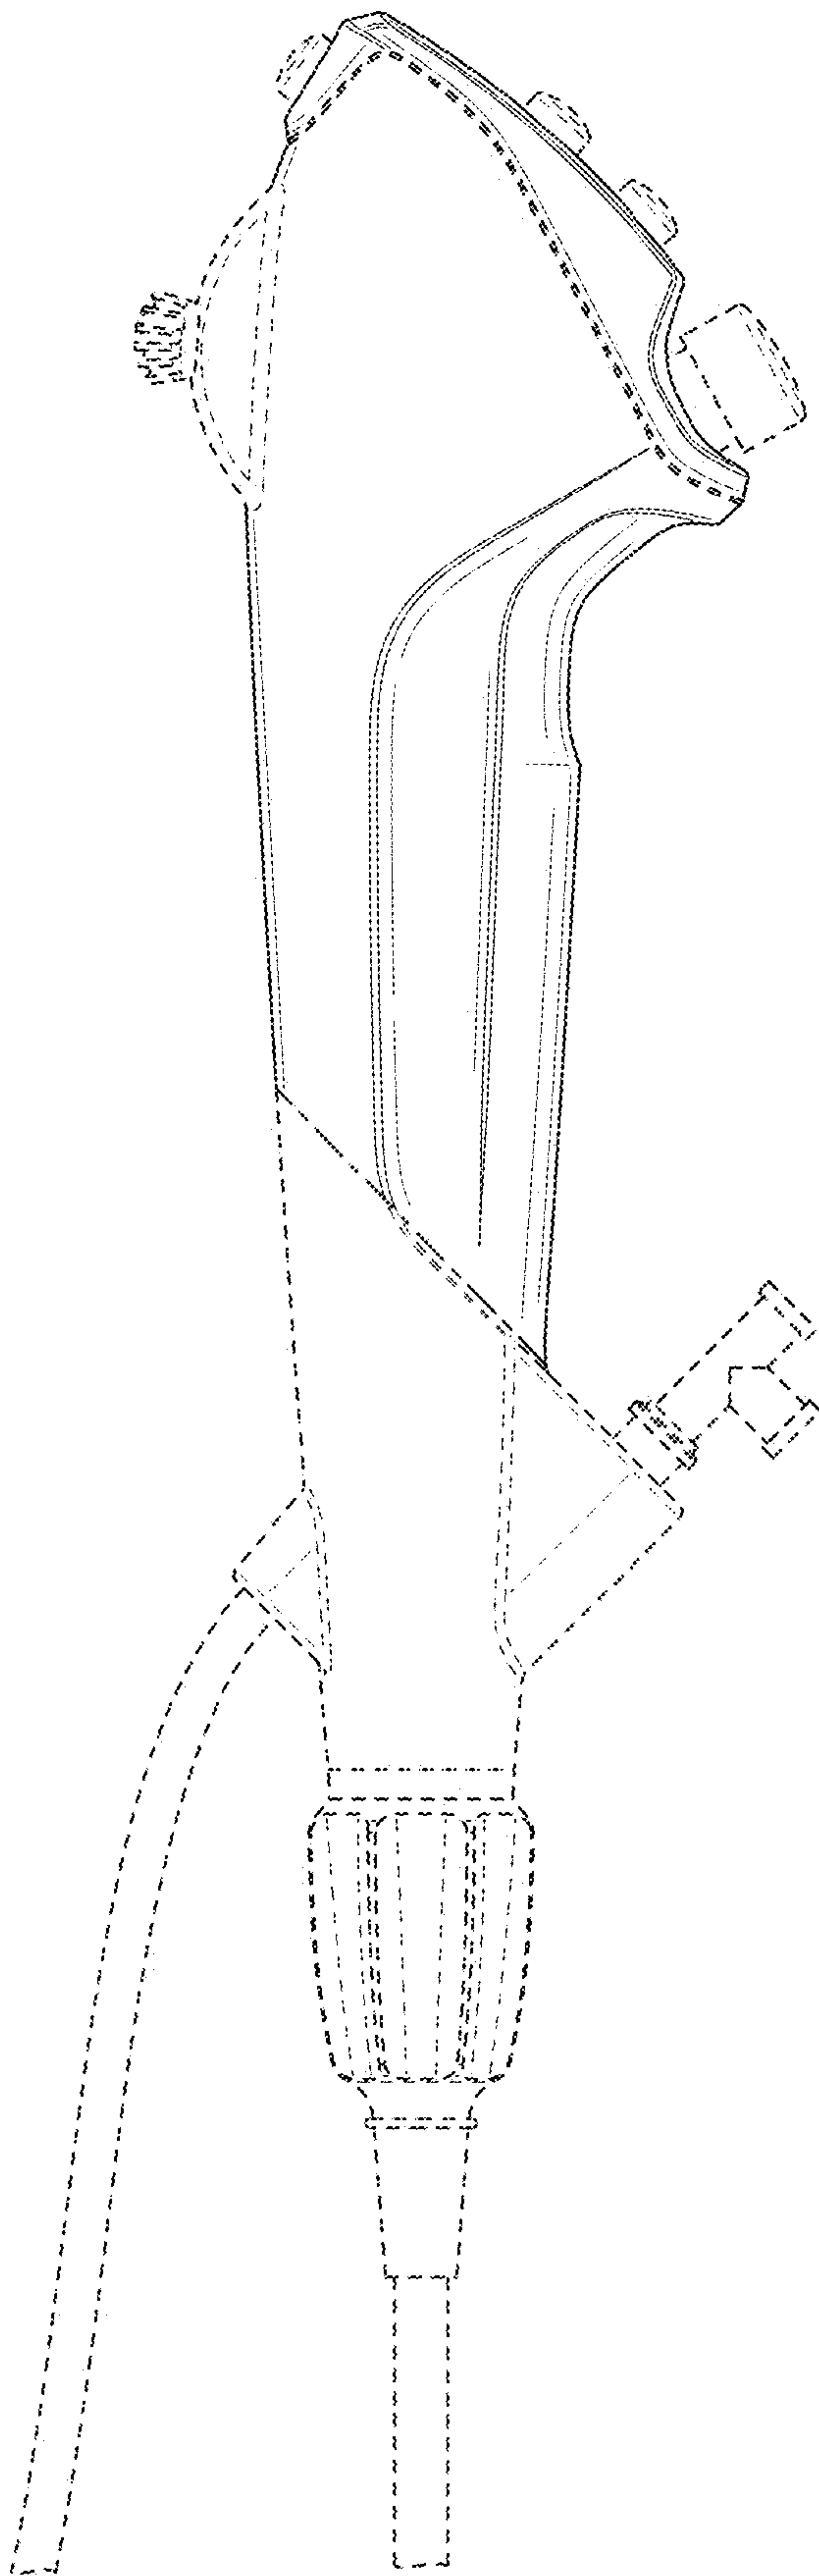


FIG. 4

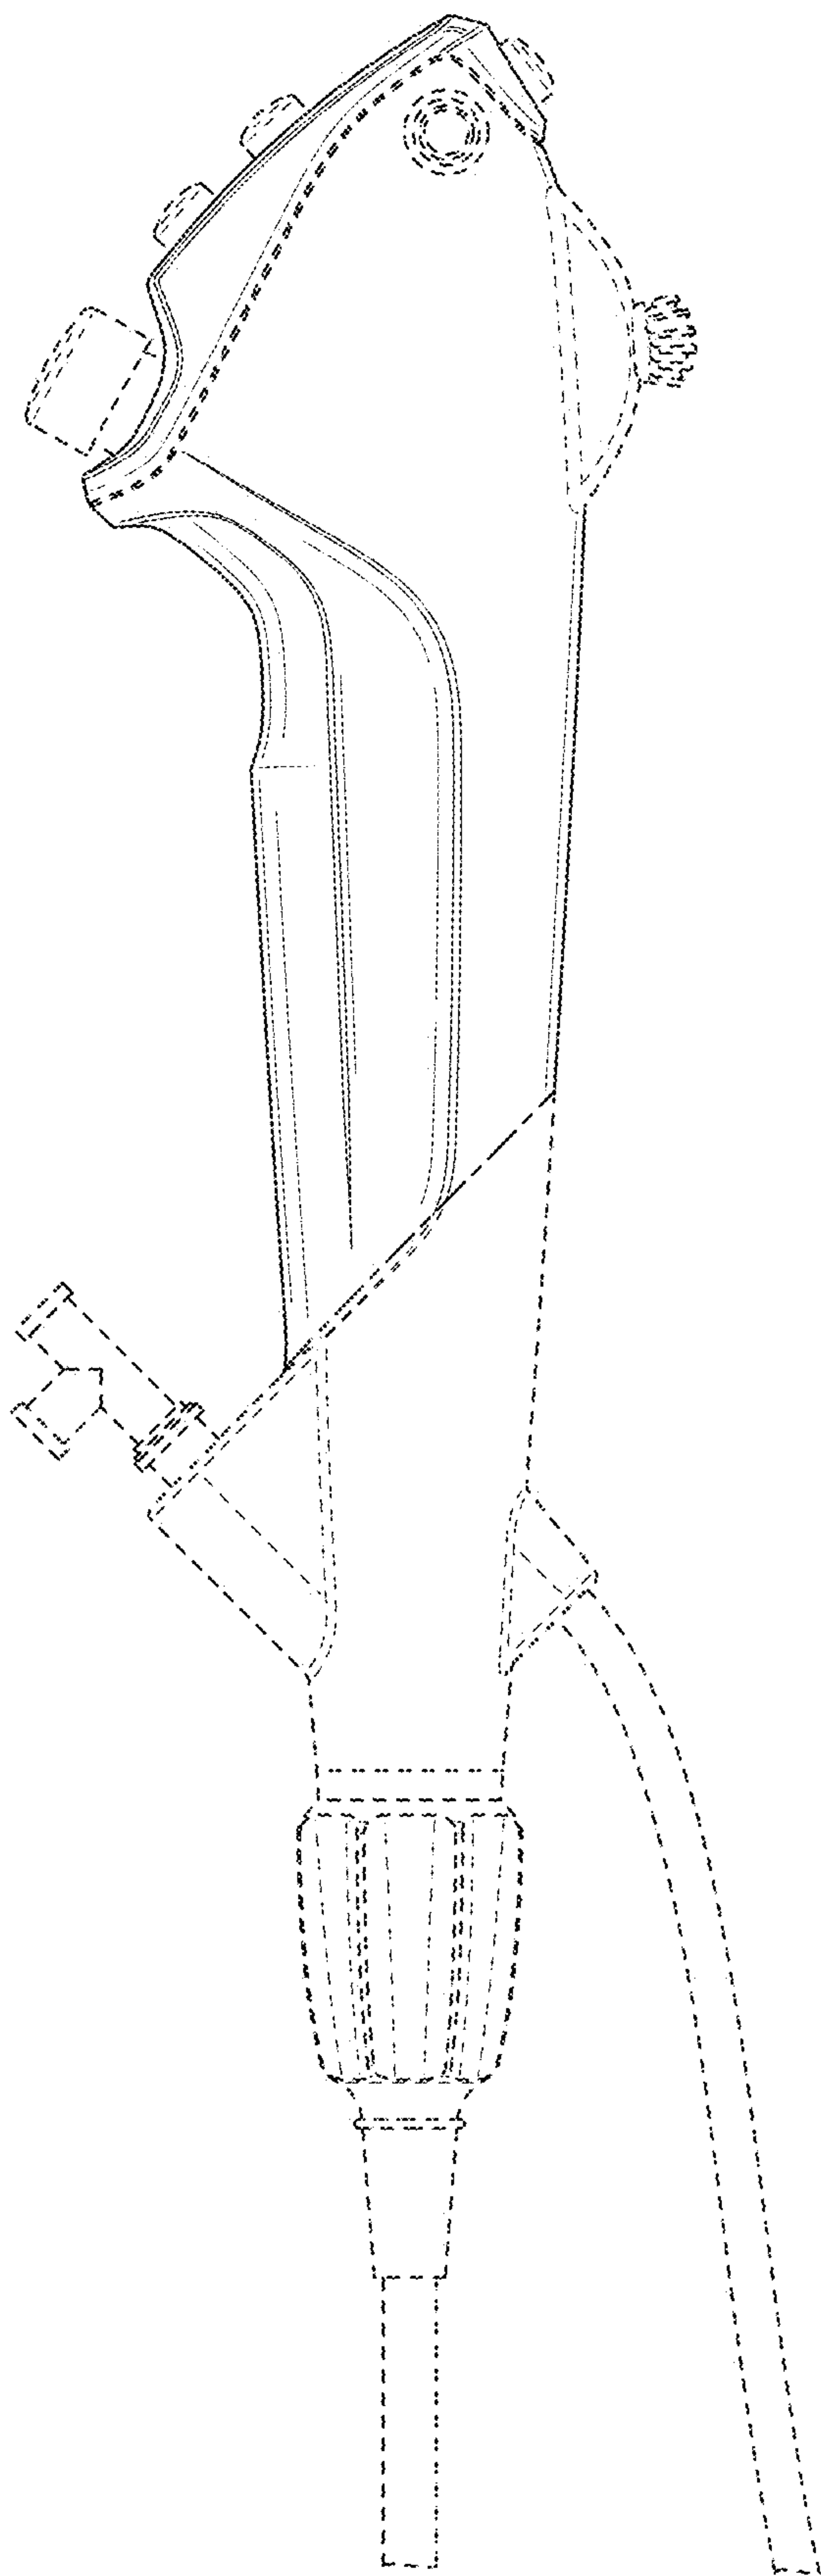


FIG. 5

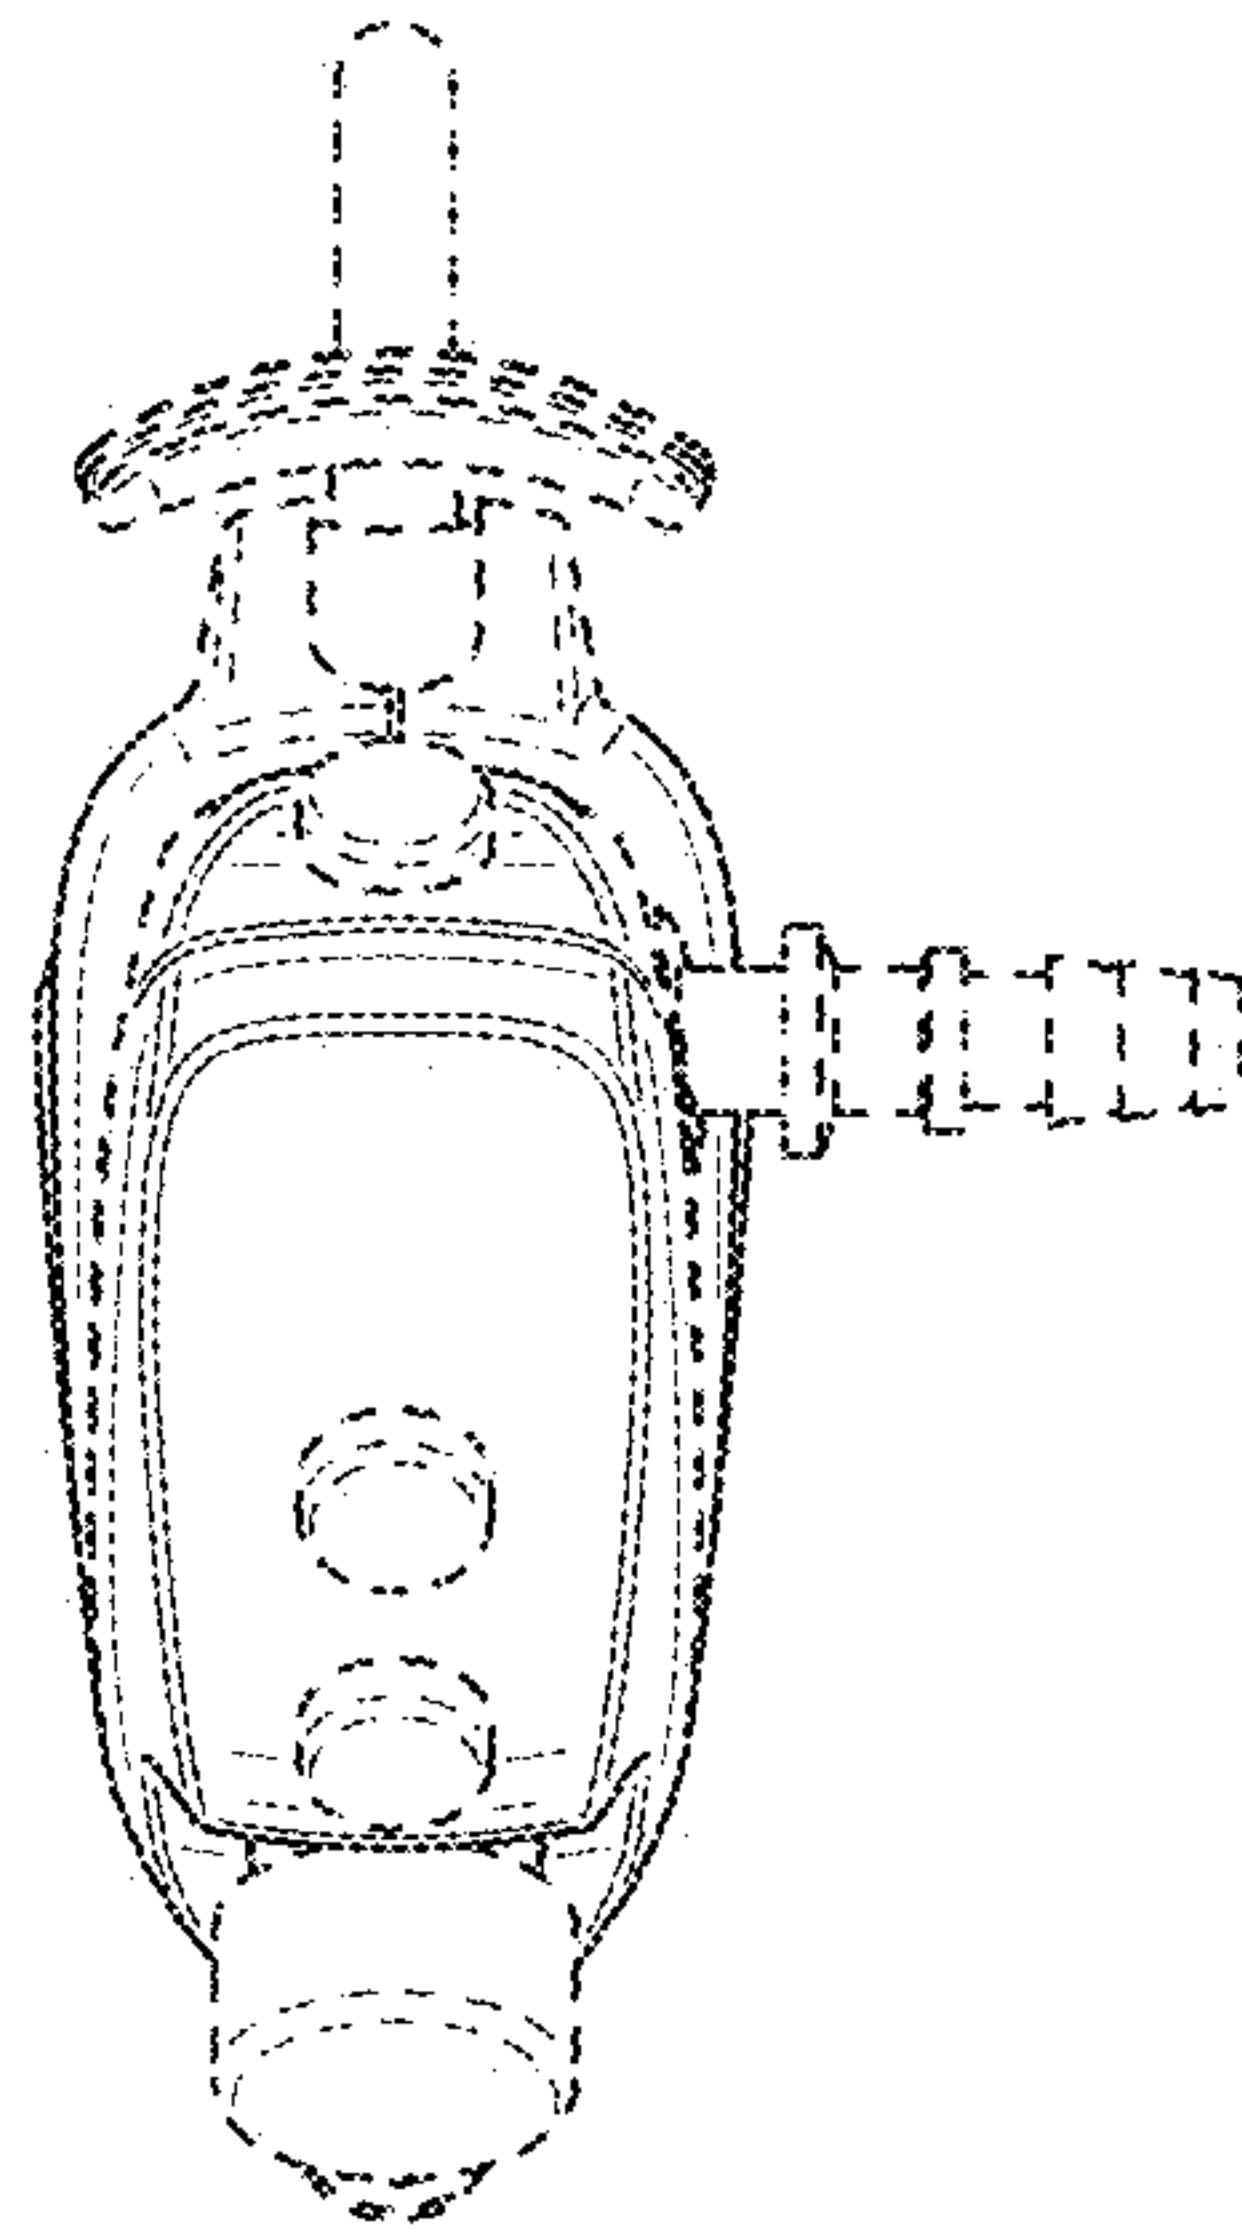


FIG. 6

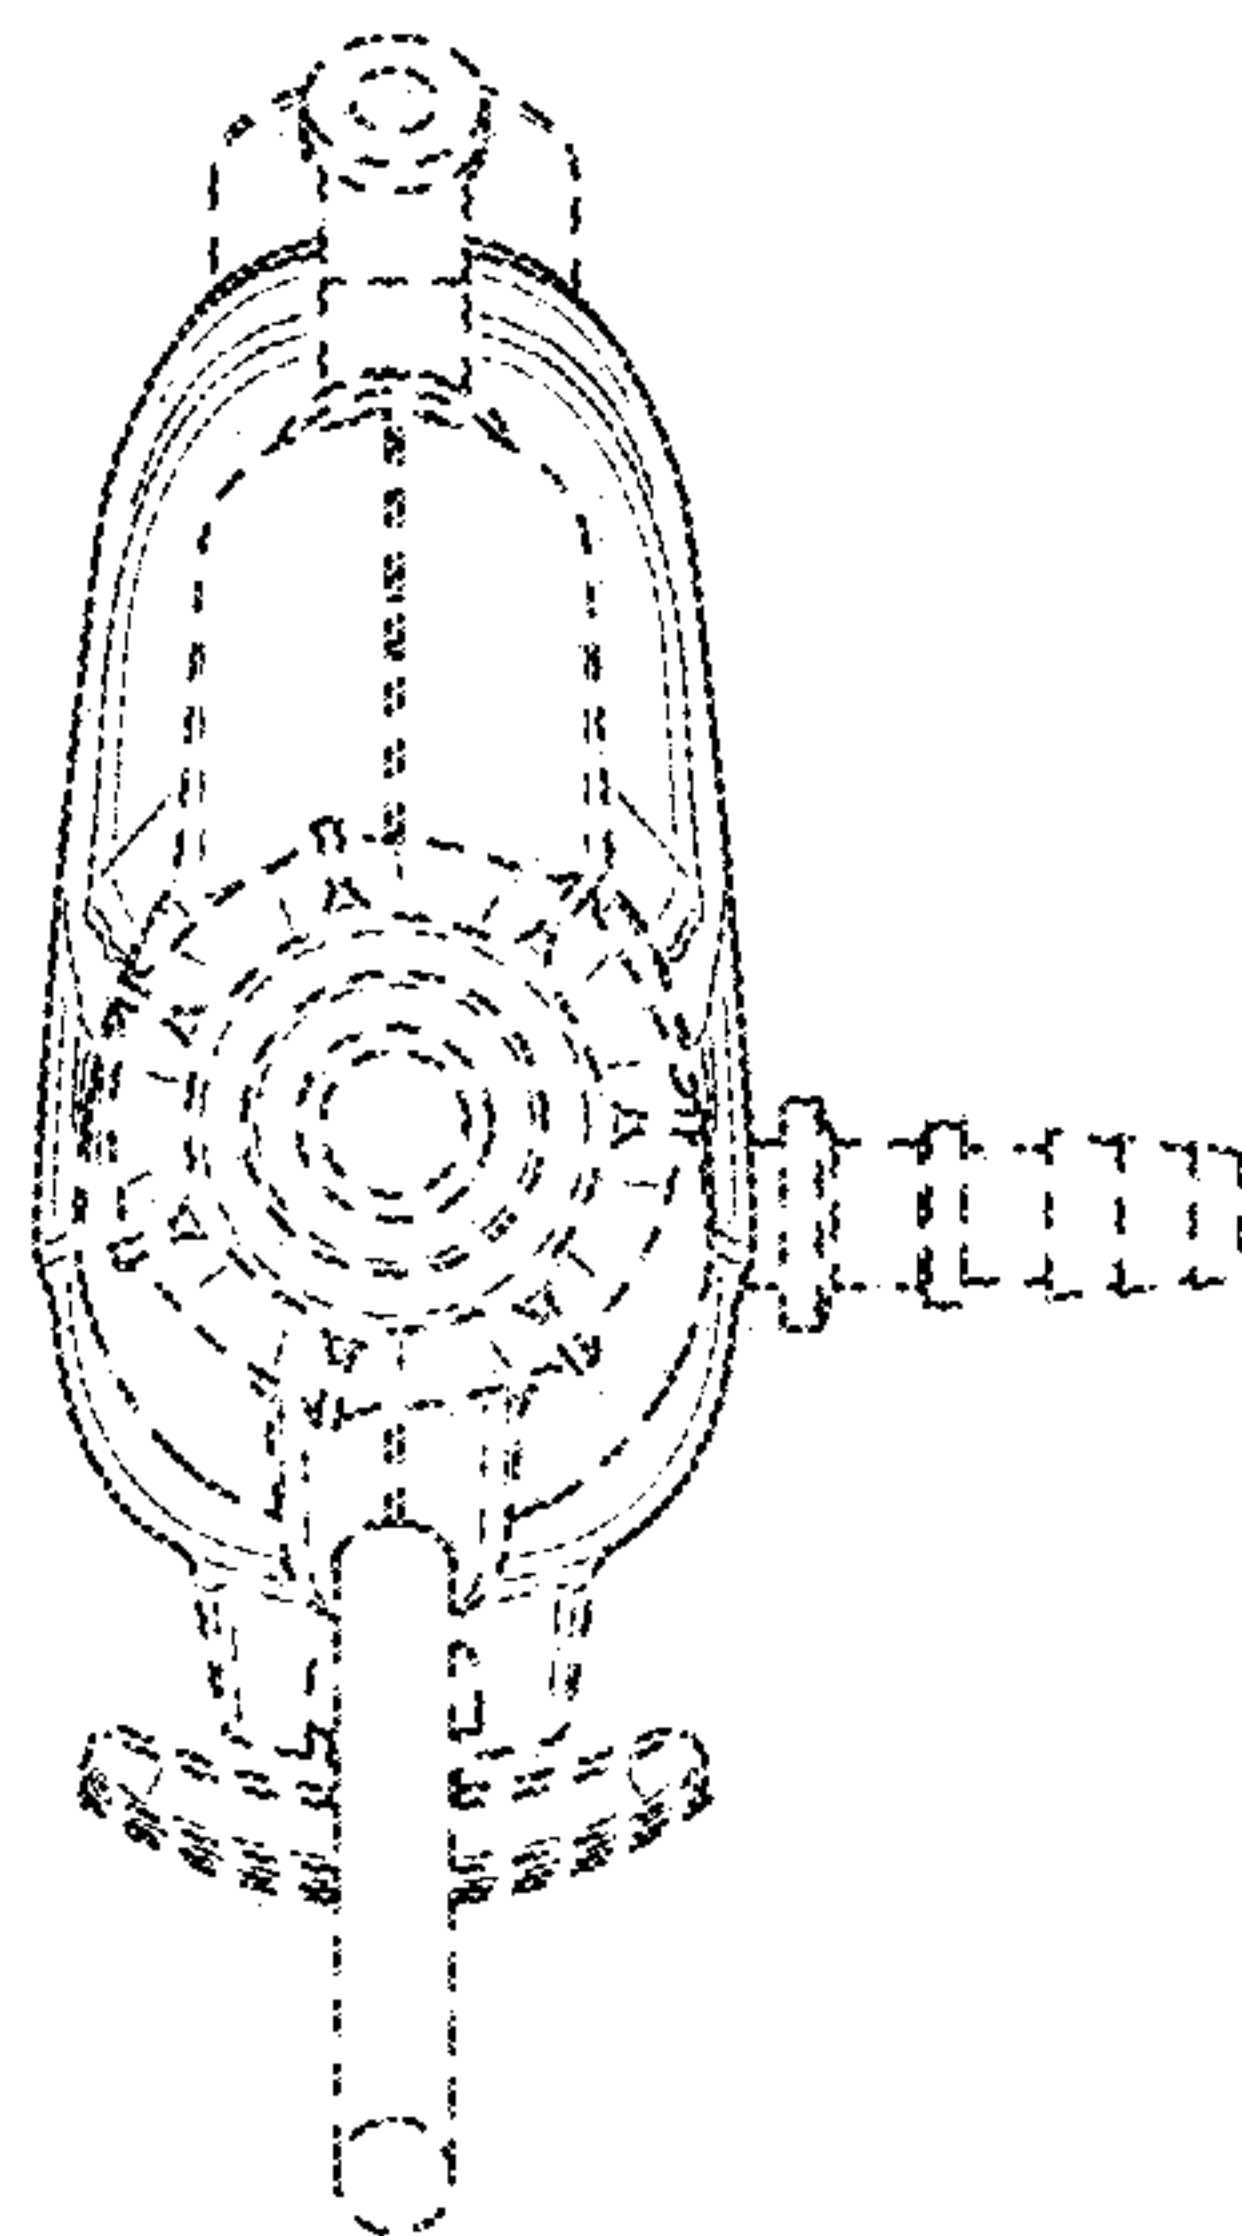


FIG. 7

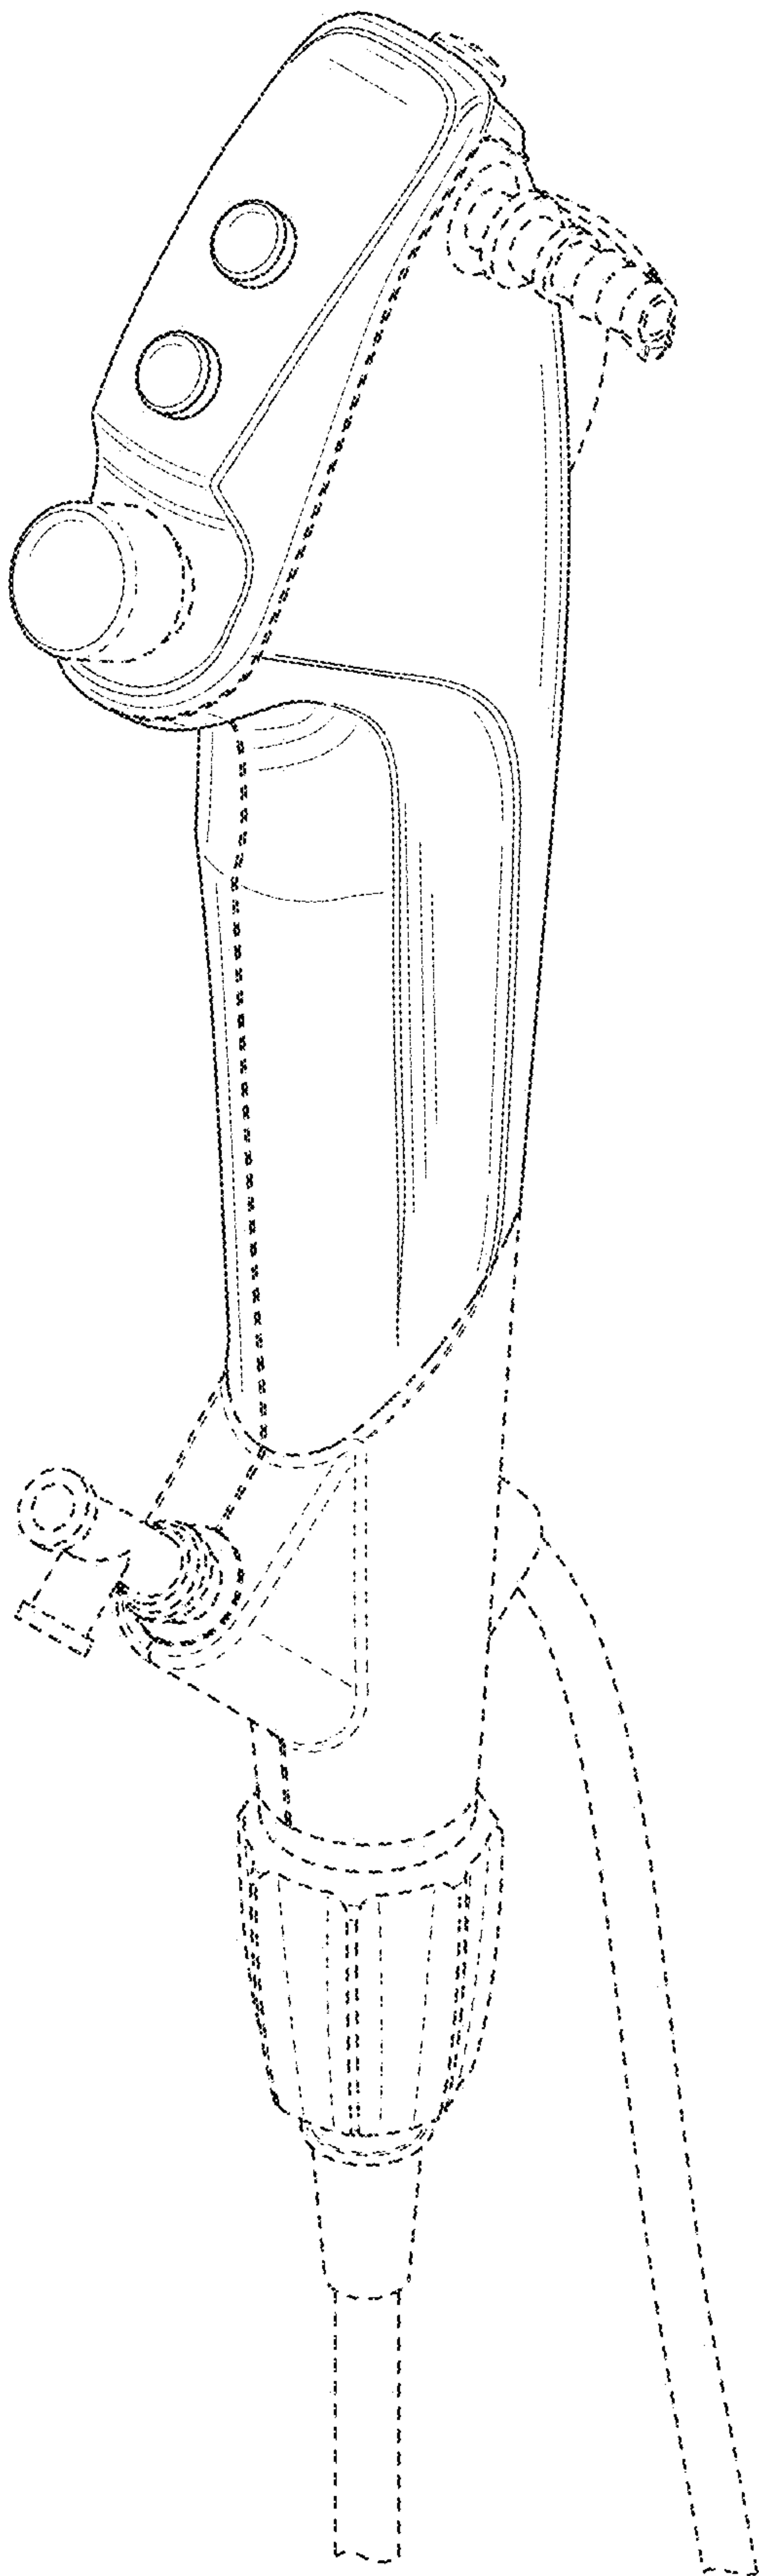


FIG. 8

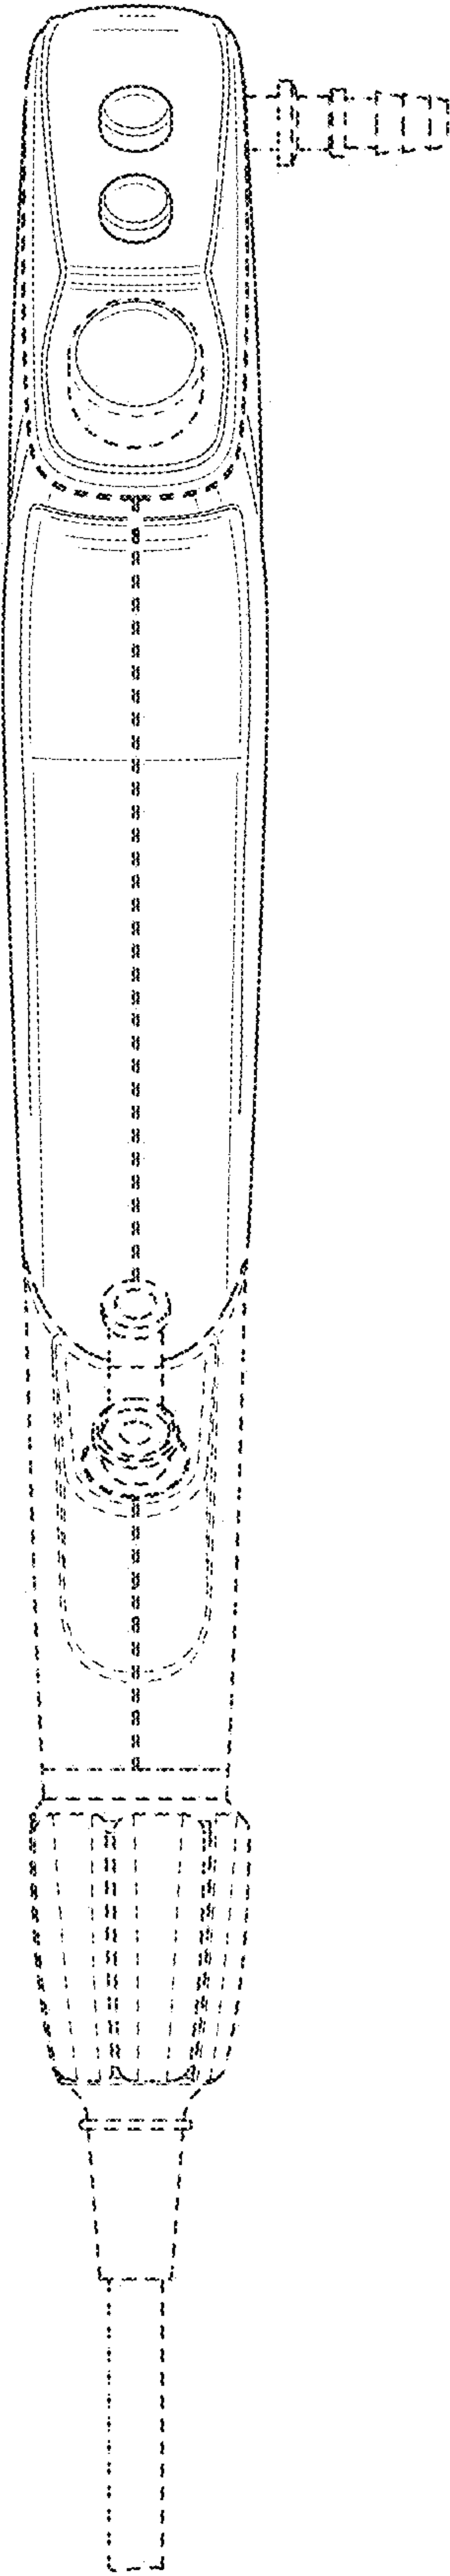


FIG. 9

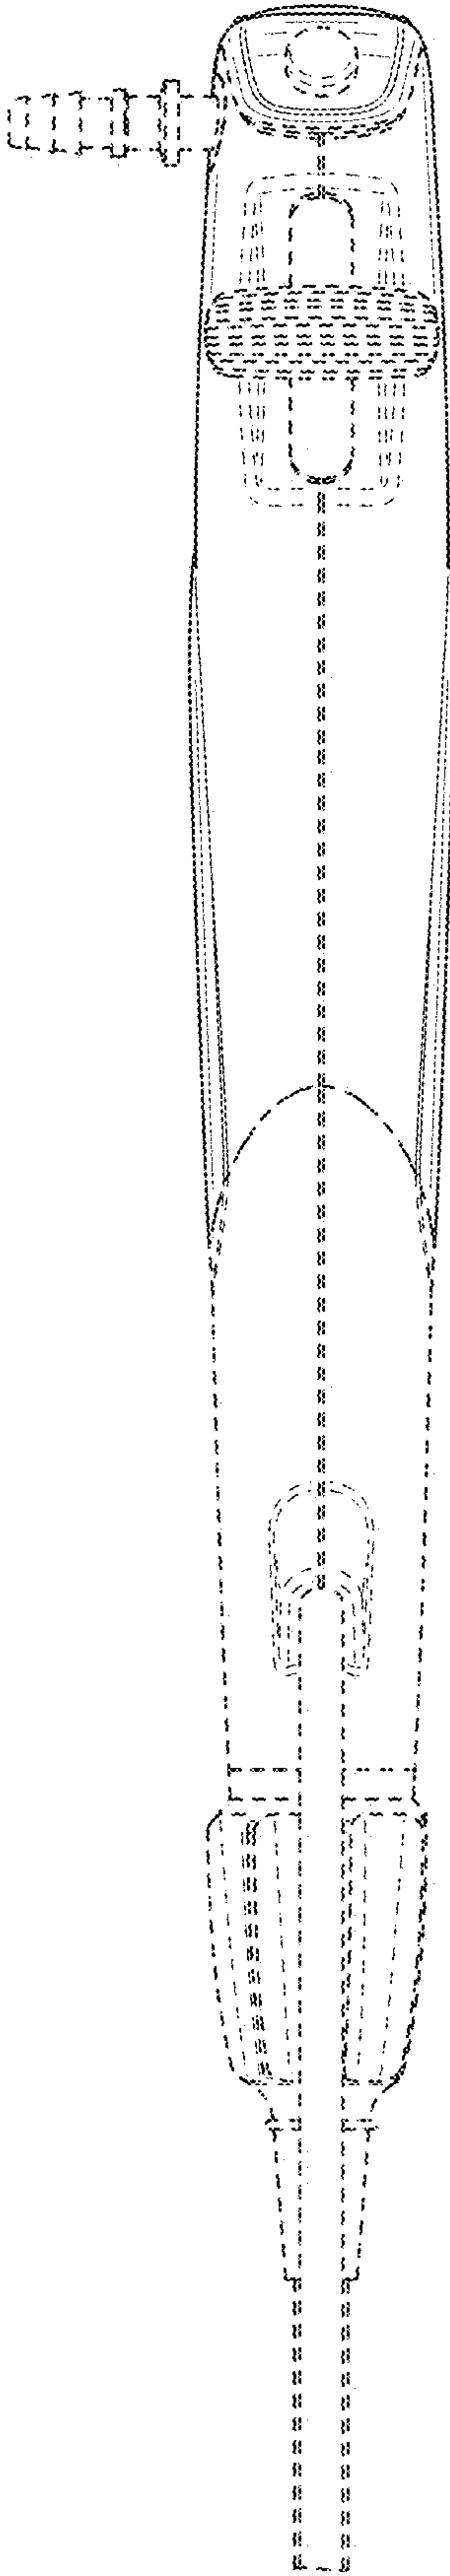


FIG. 10

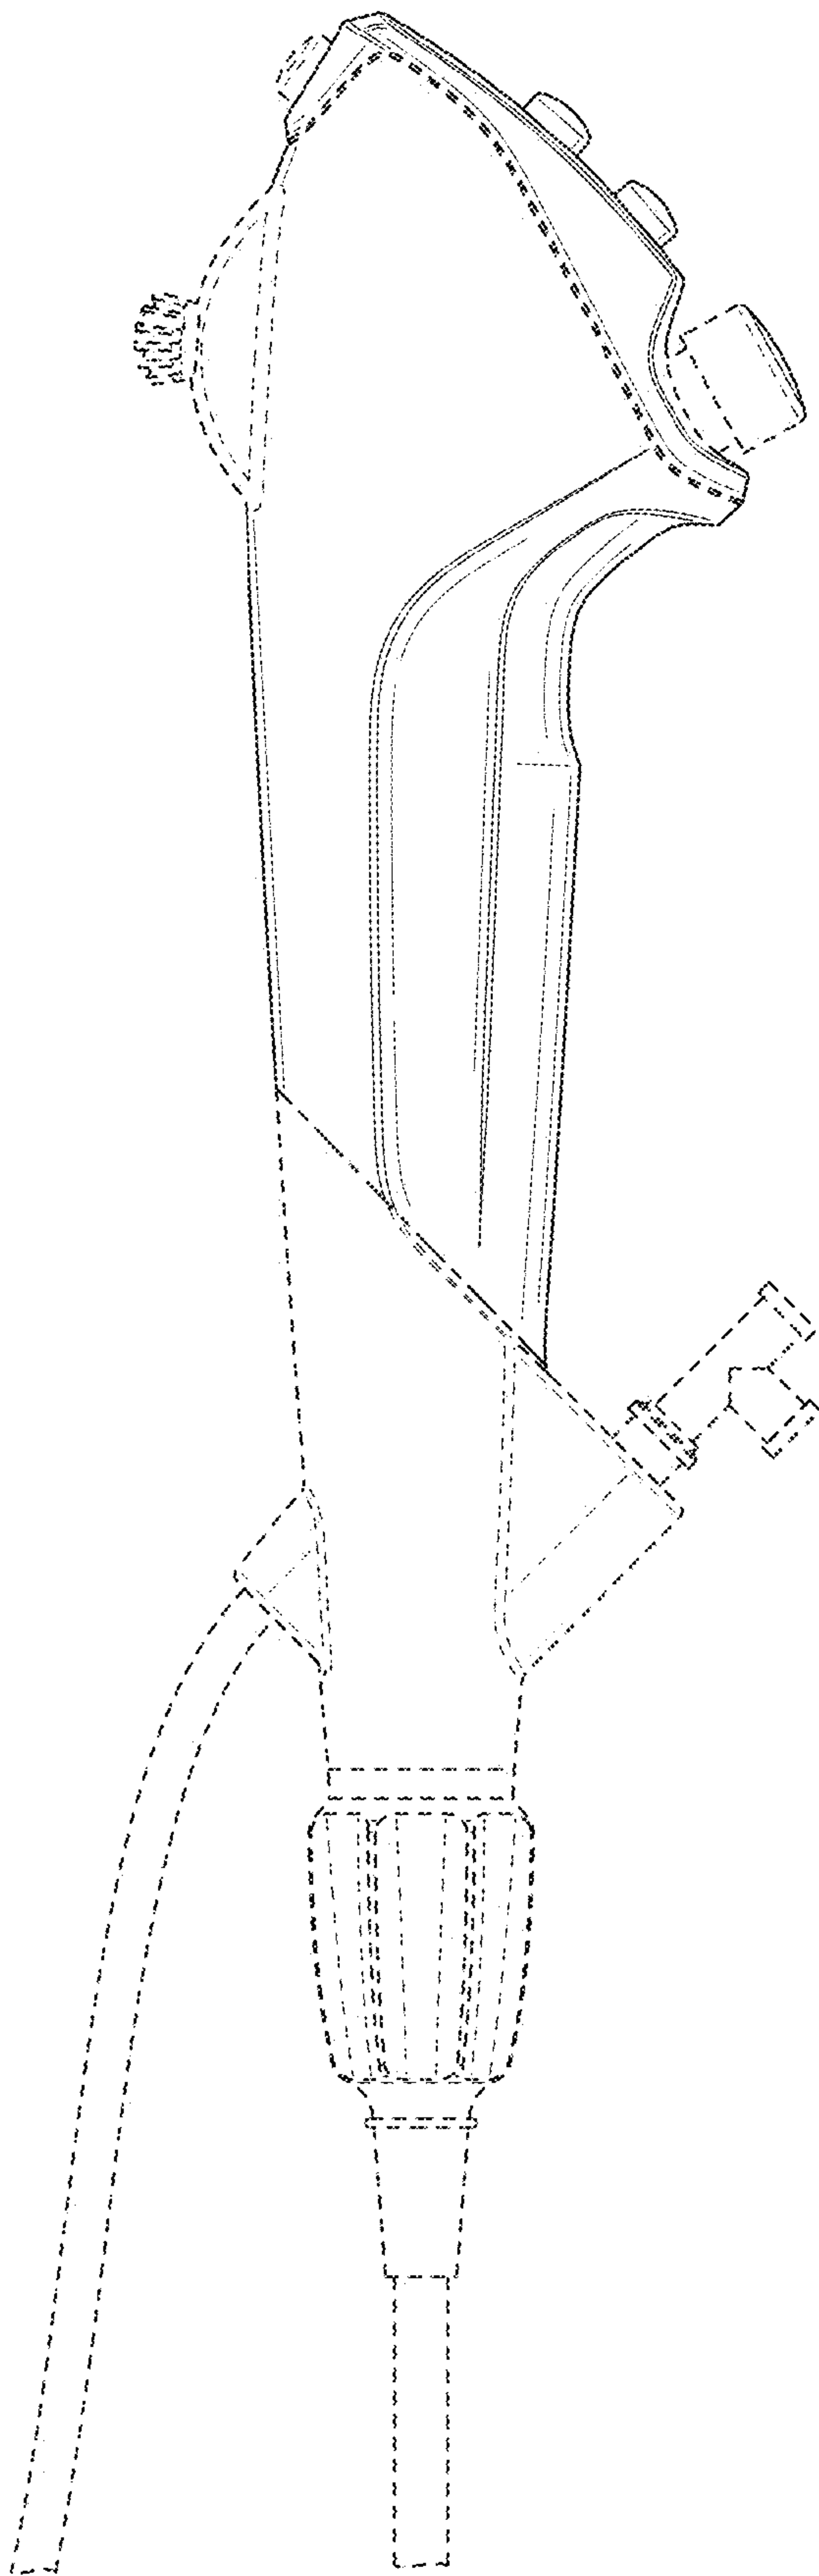


FIG. 11

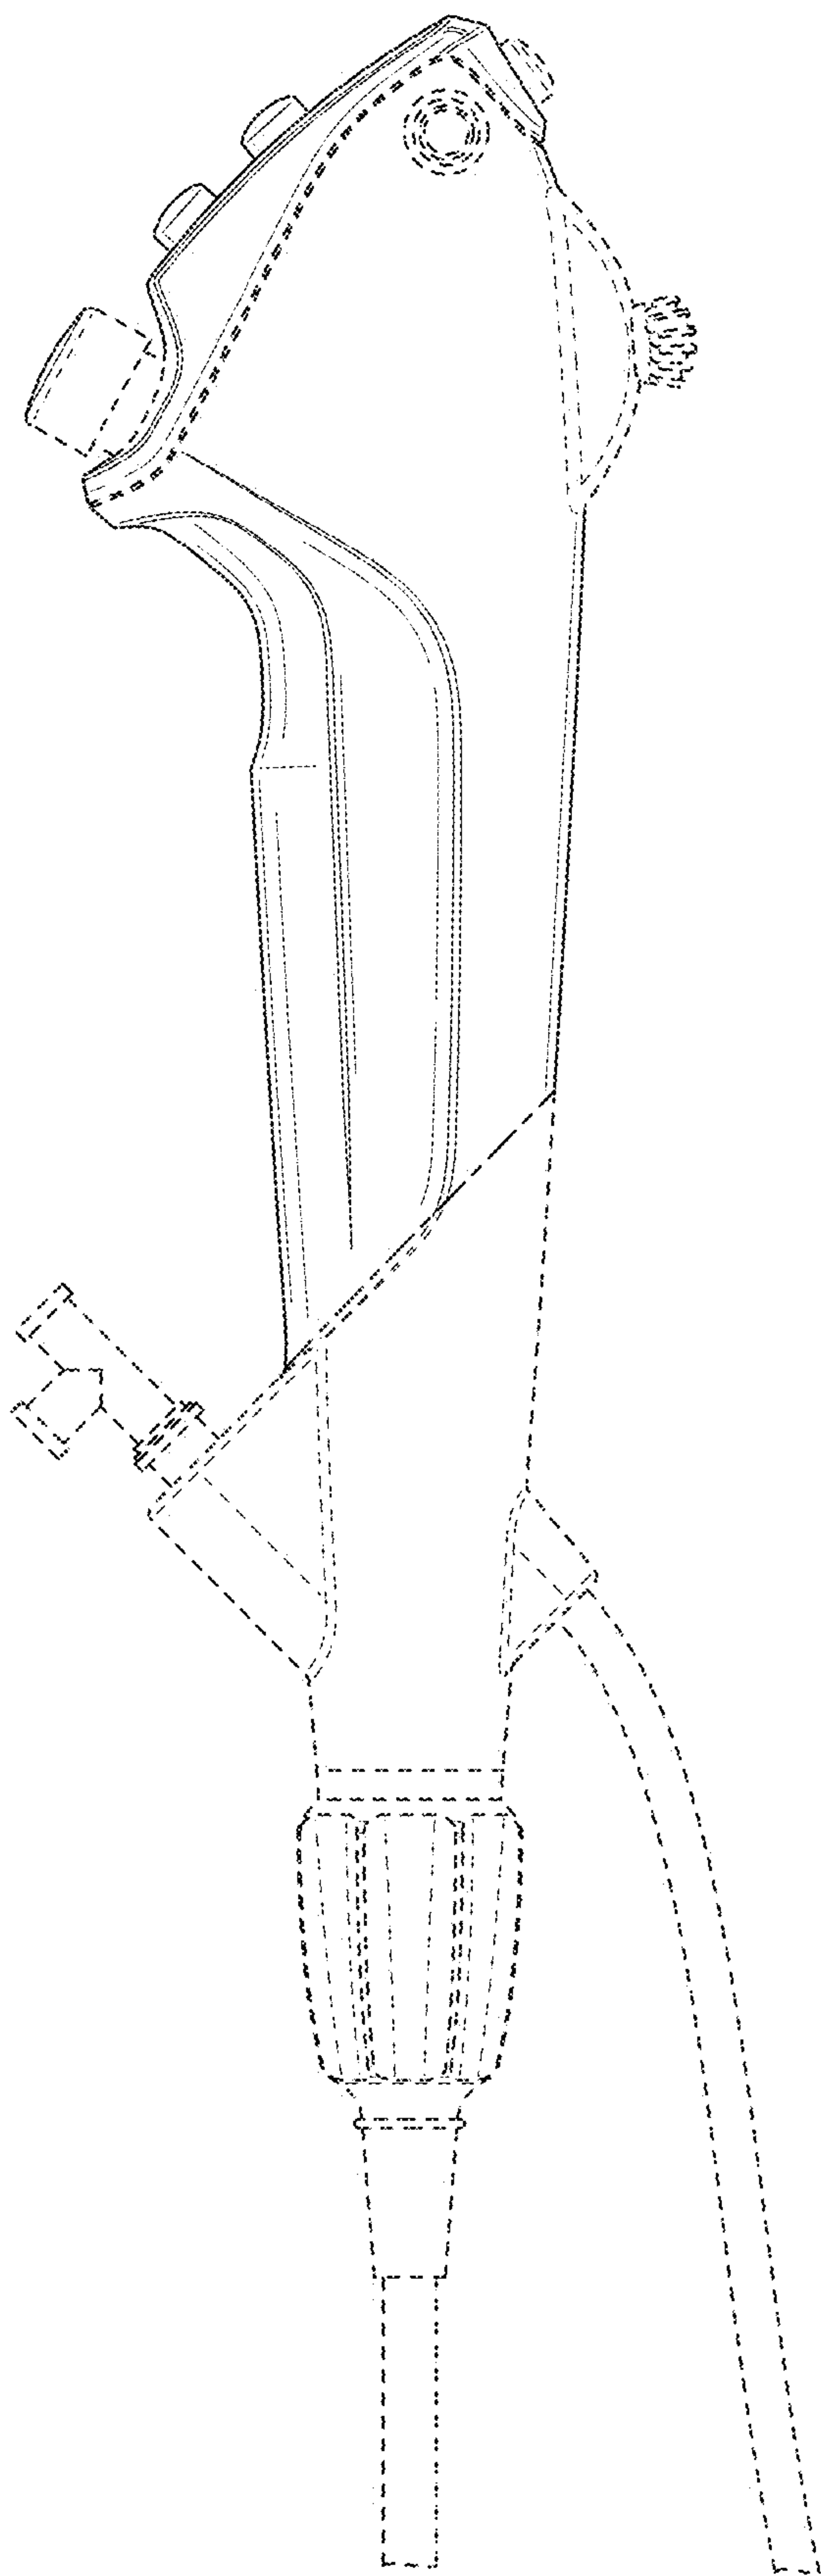


FIG. 12

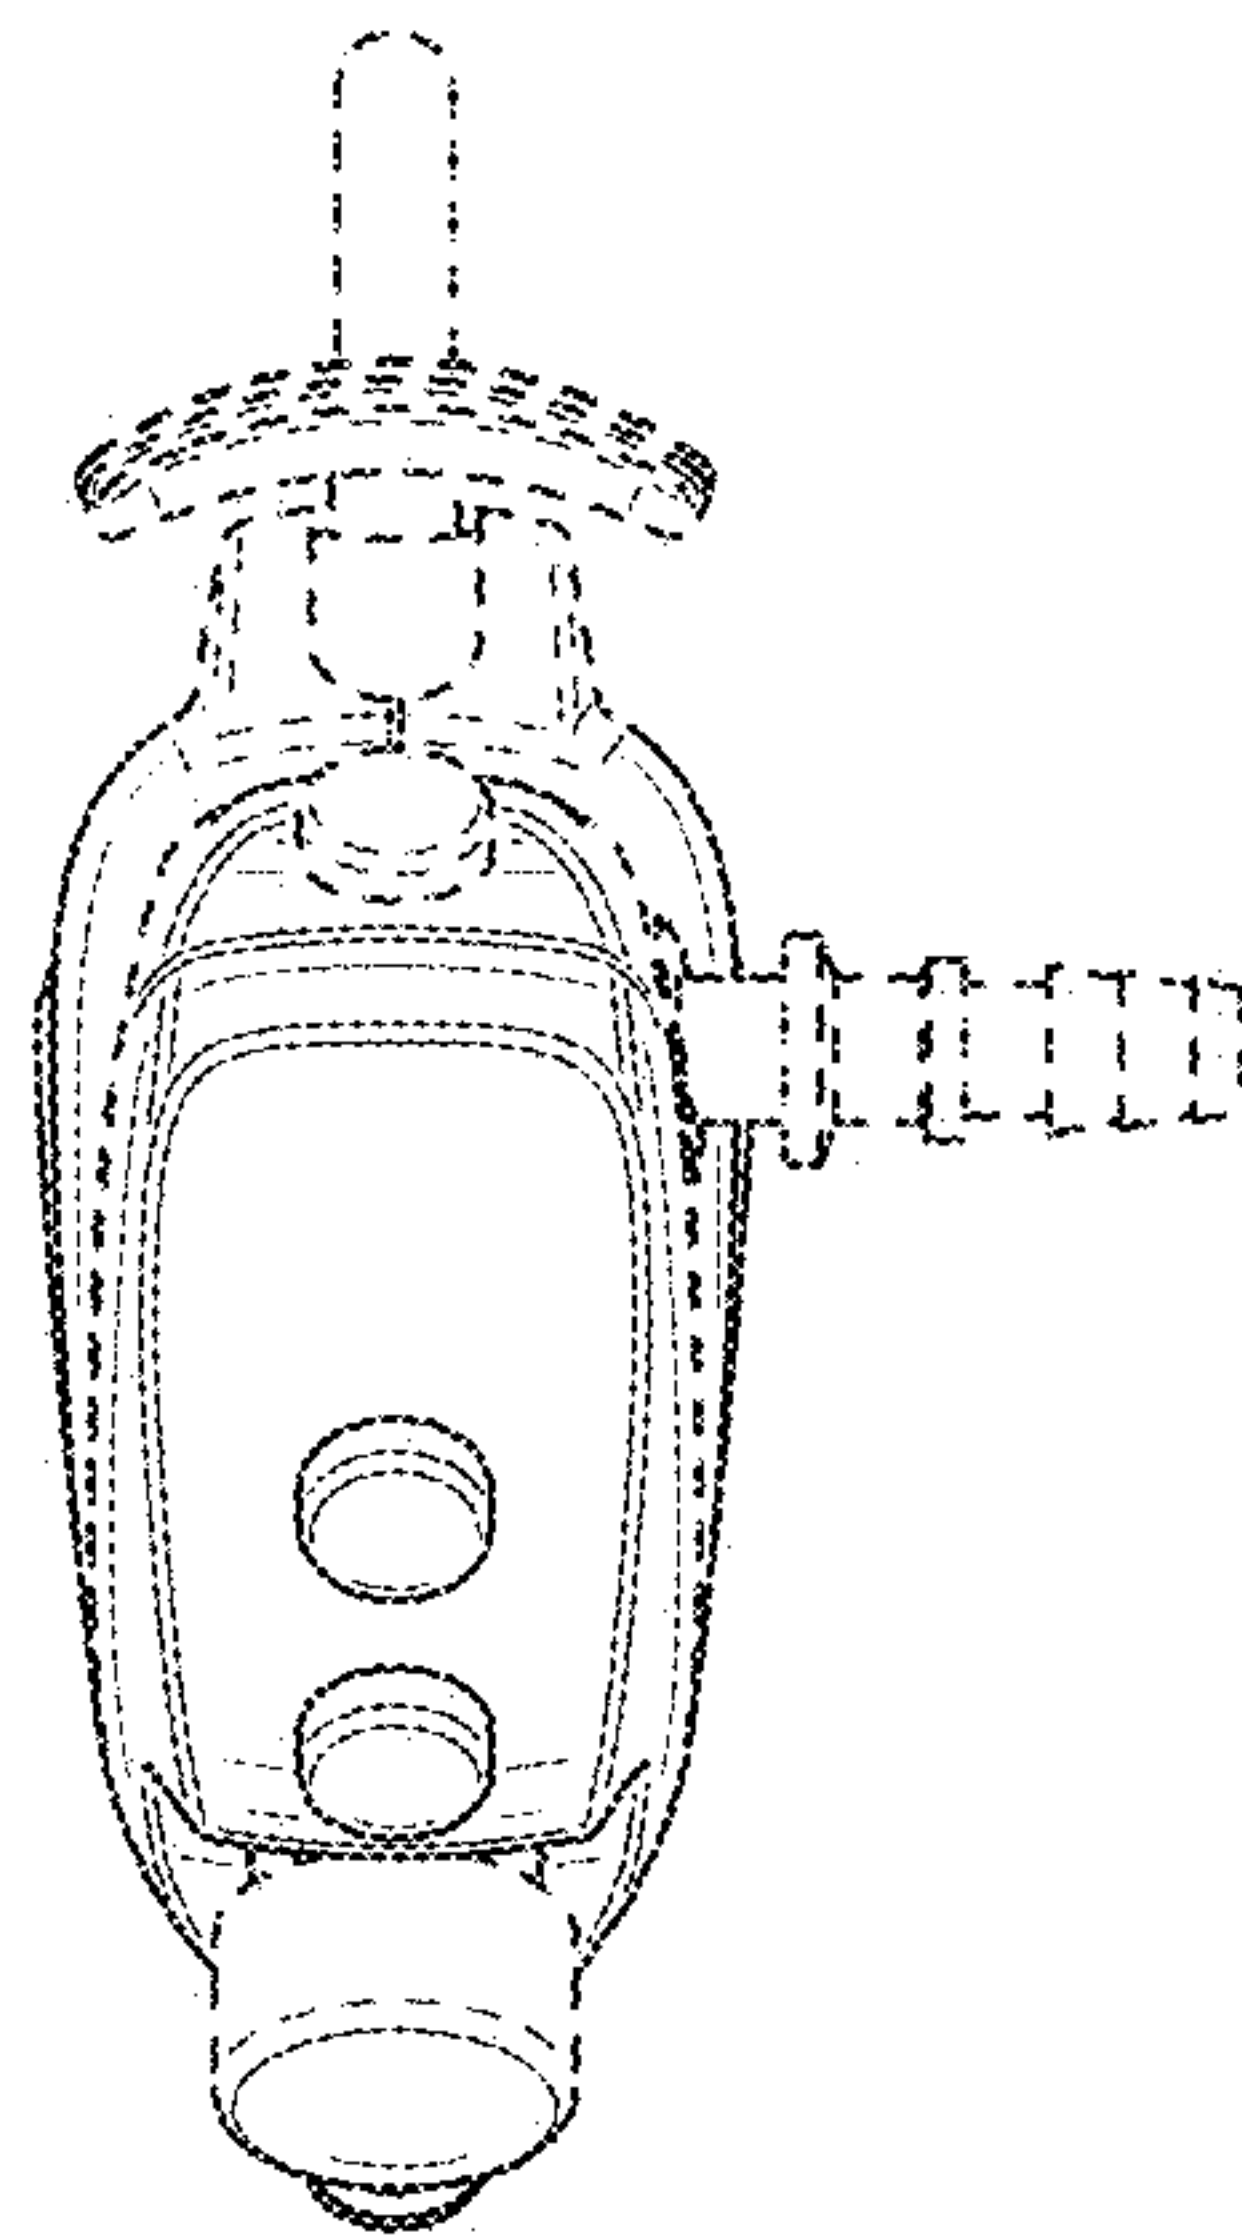


FIG. 13

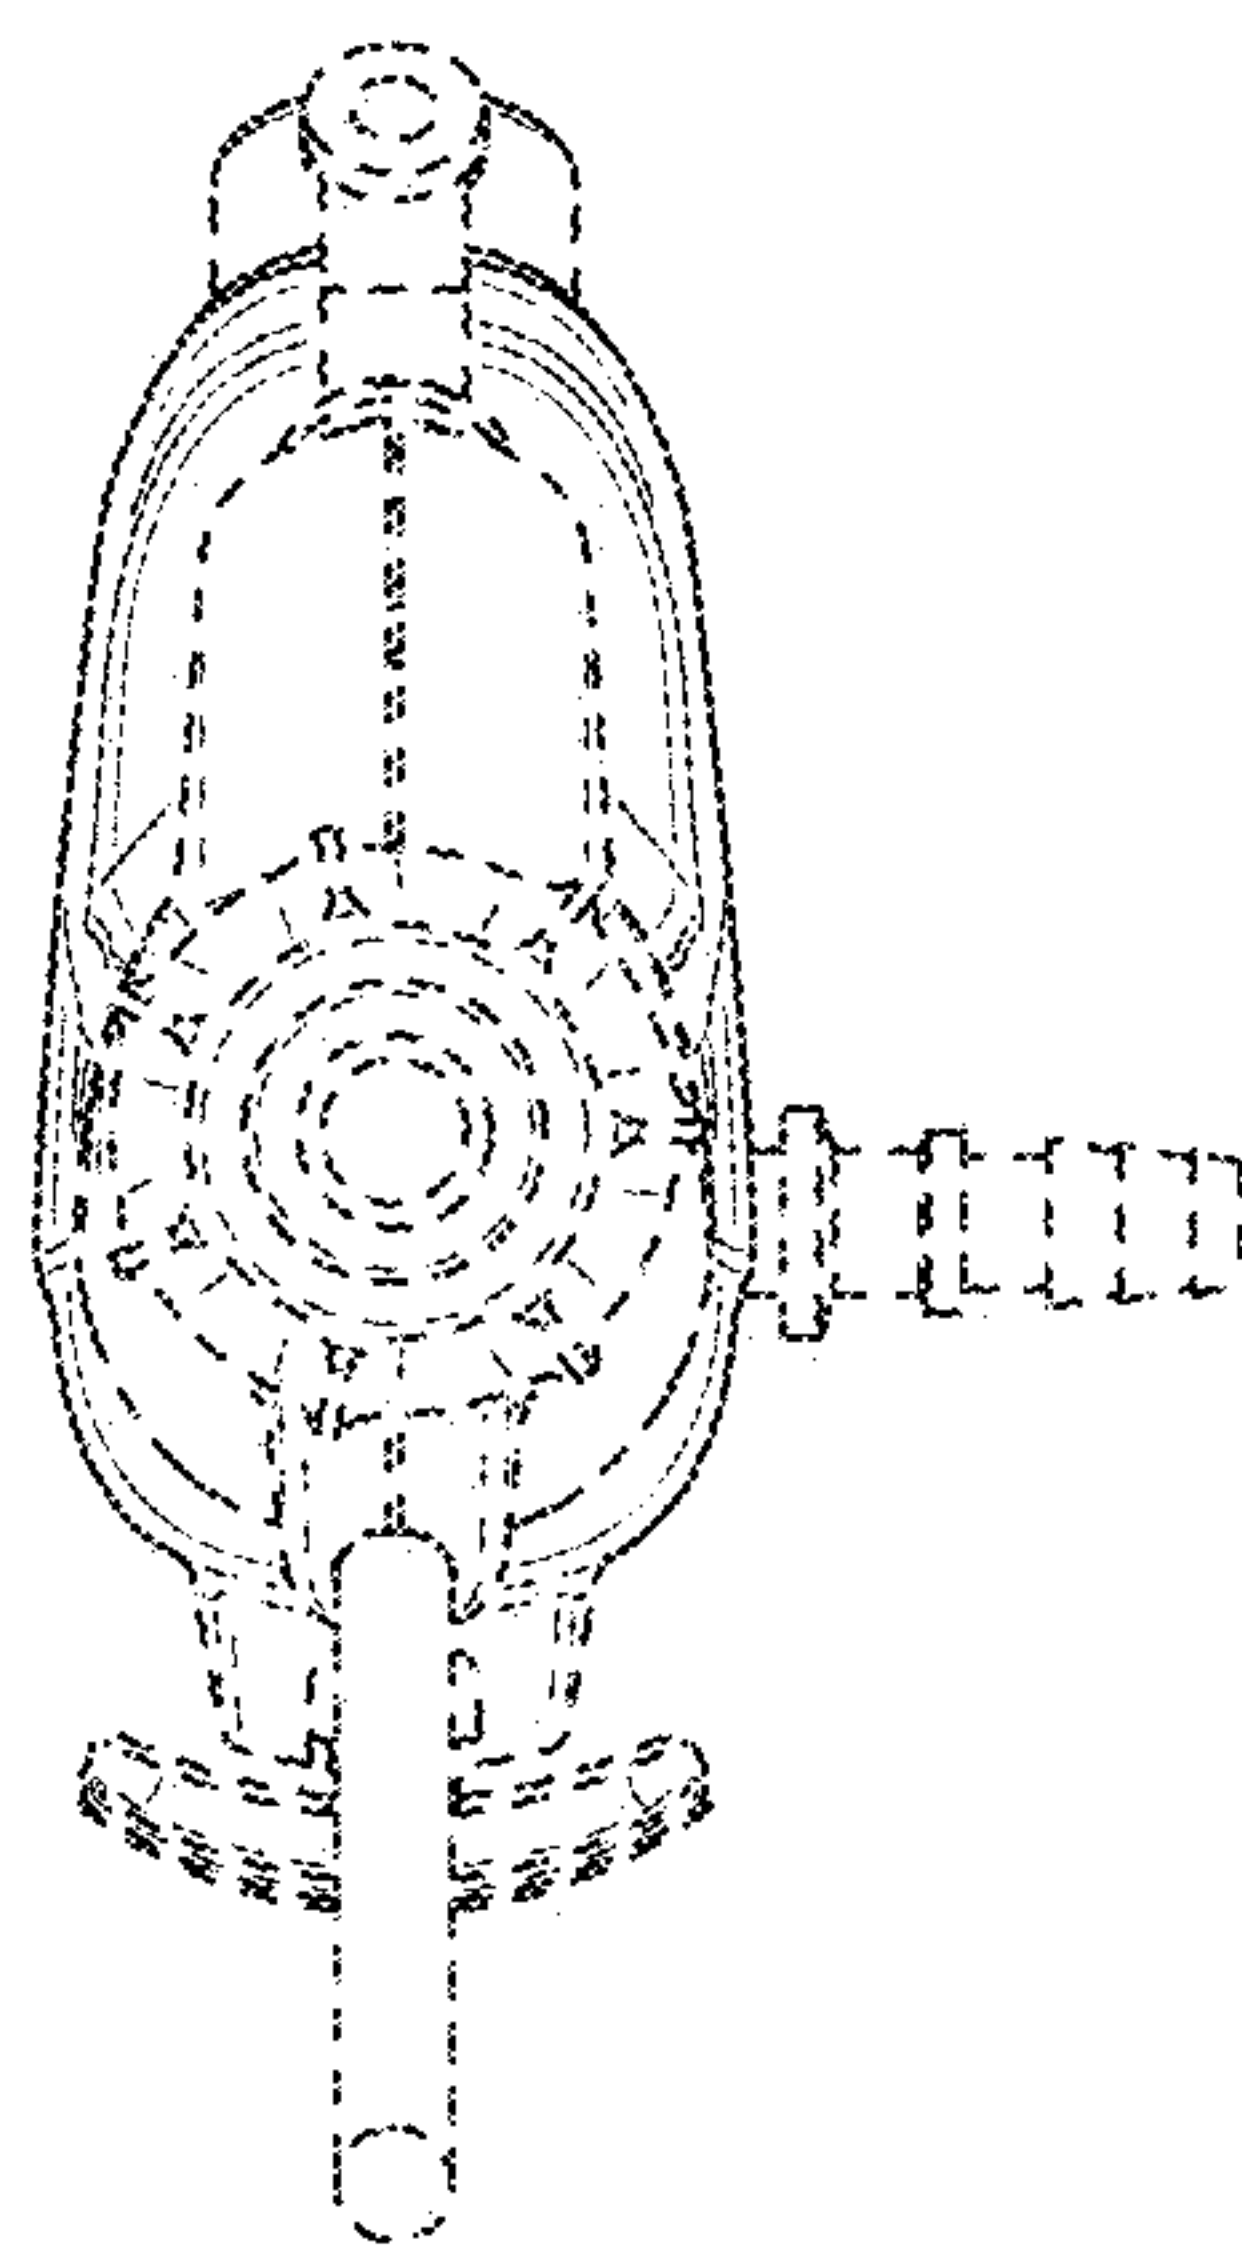


FIG. 14

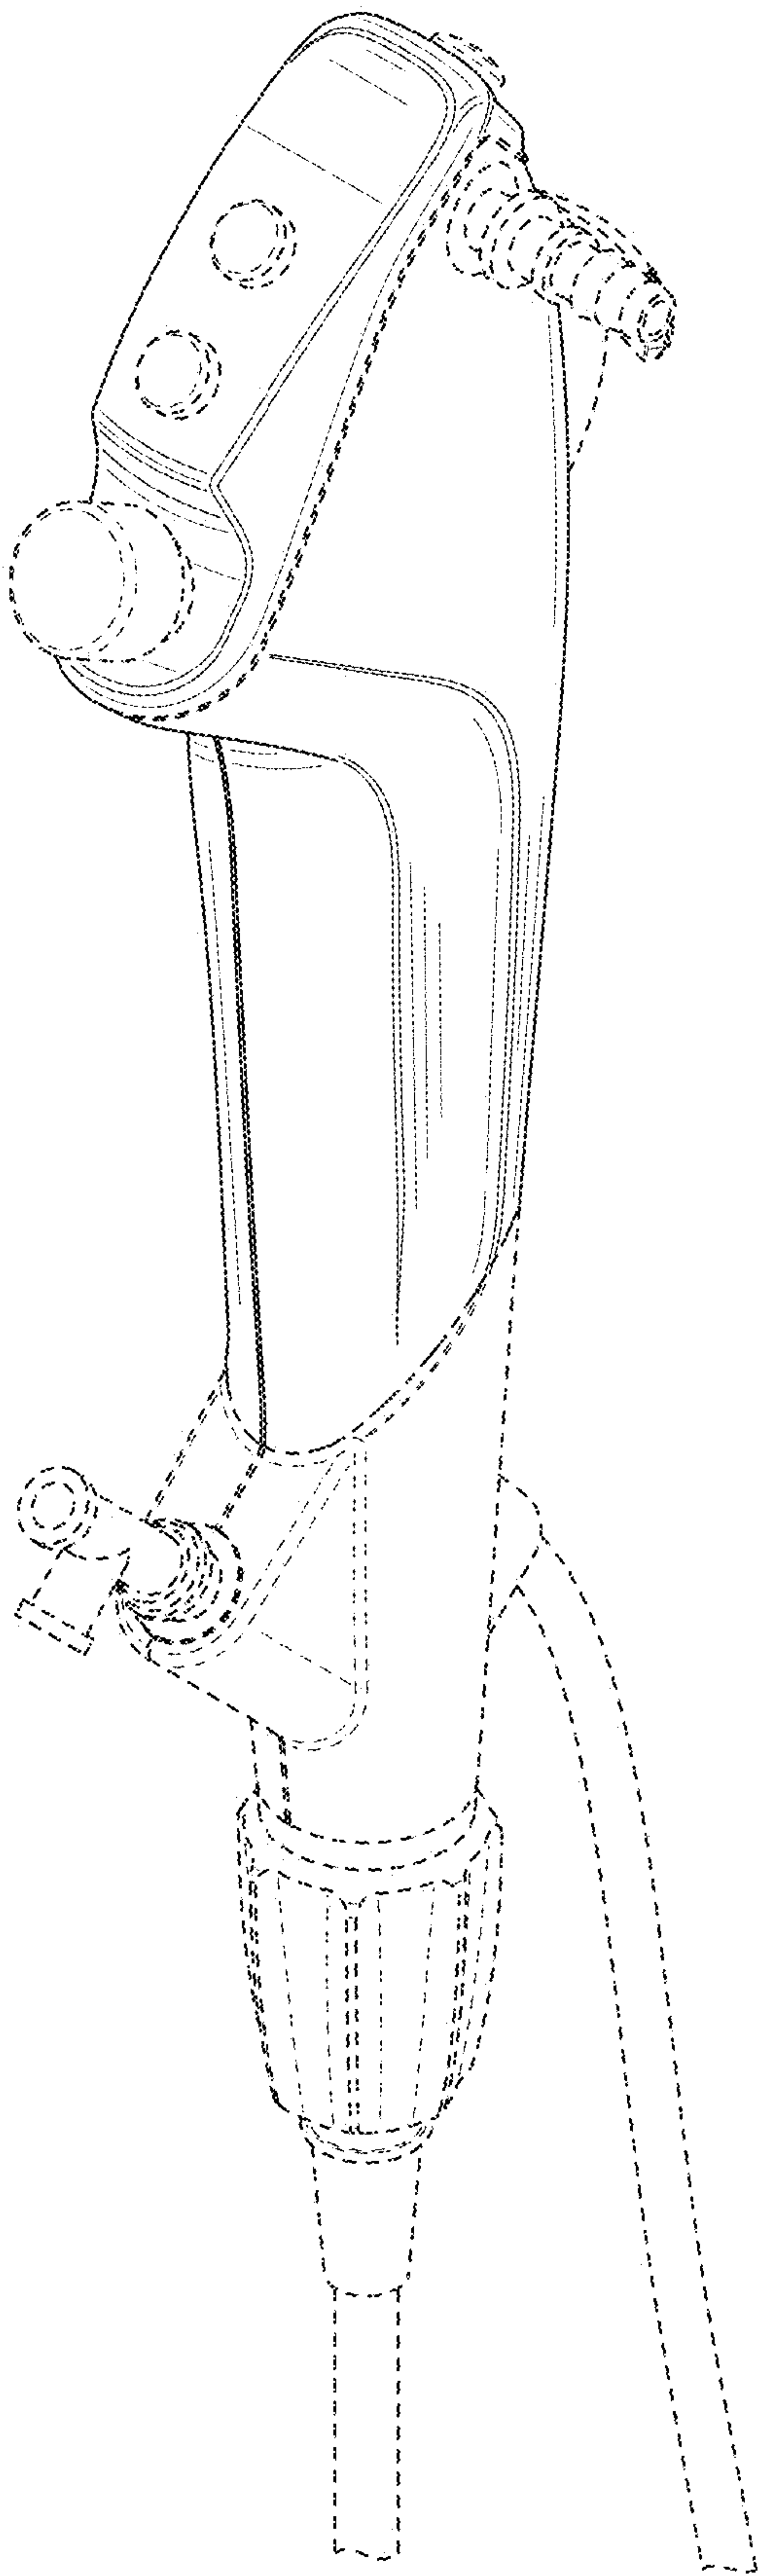


FIG. 15

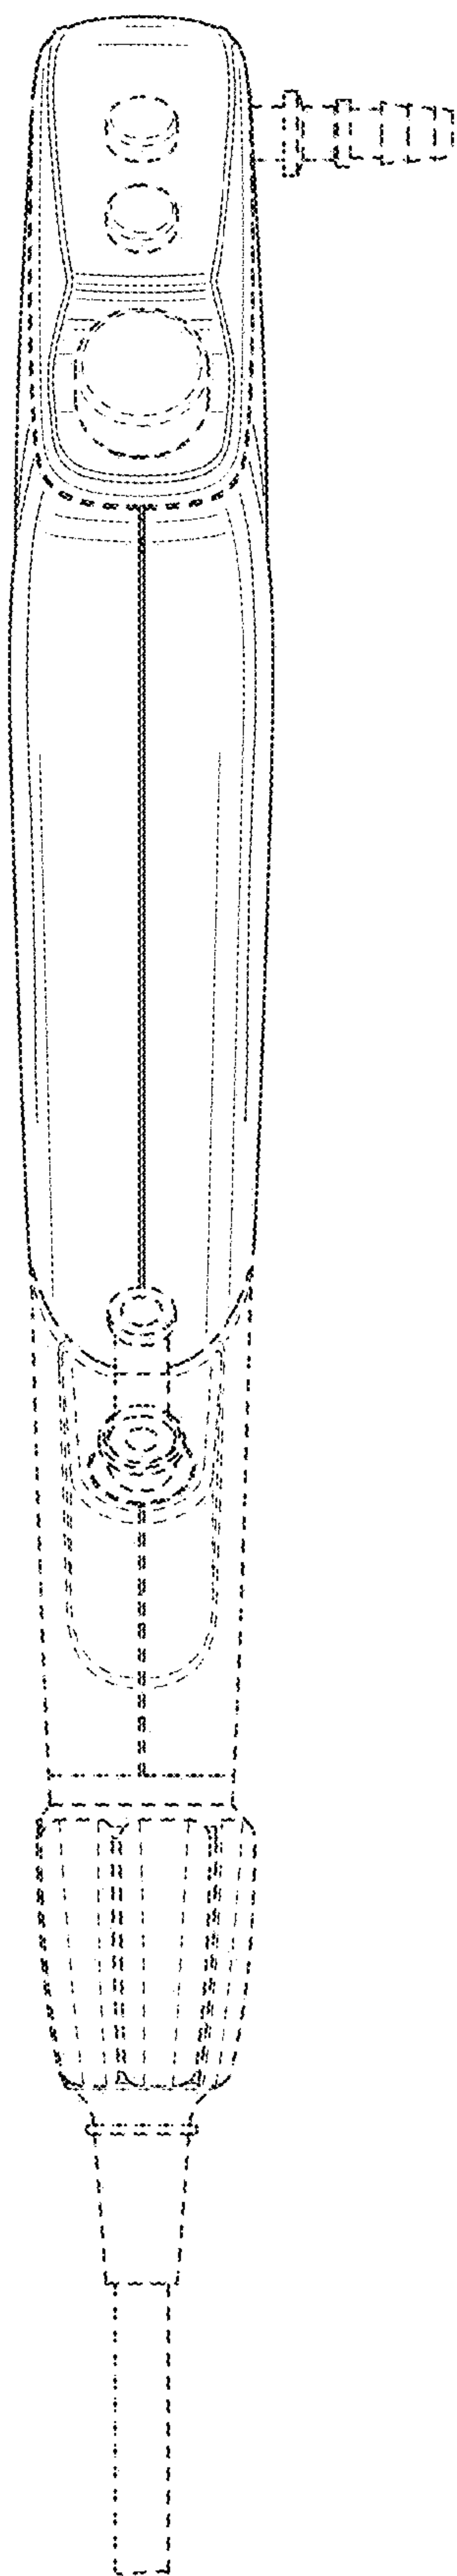


FIG. 16

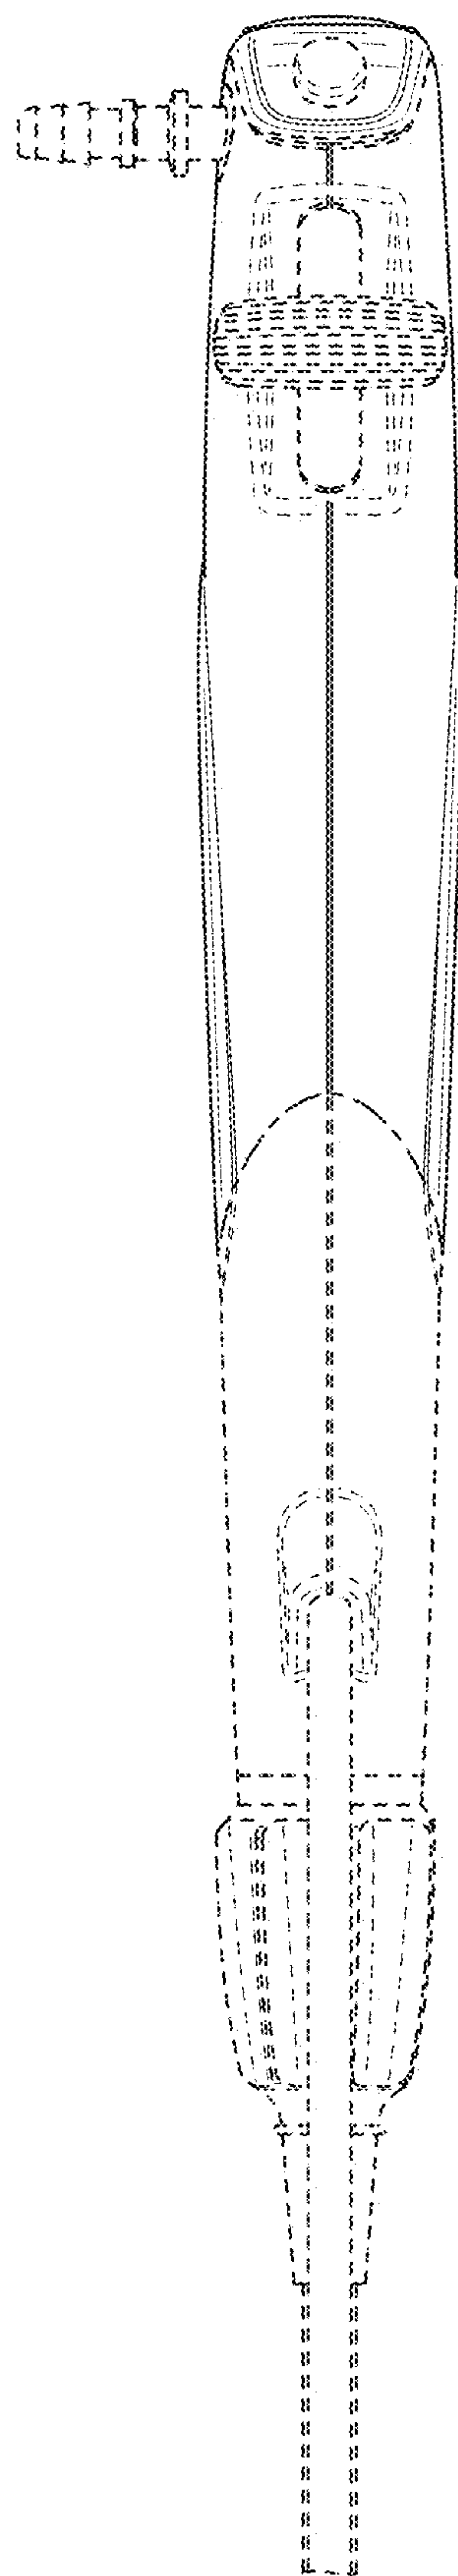


FIG. 17

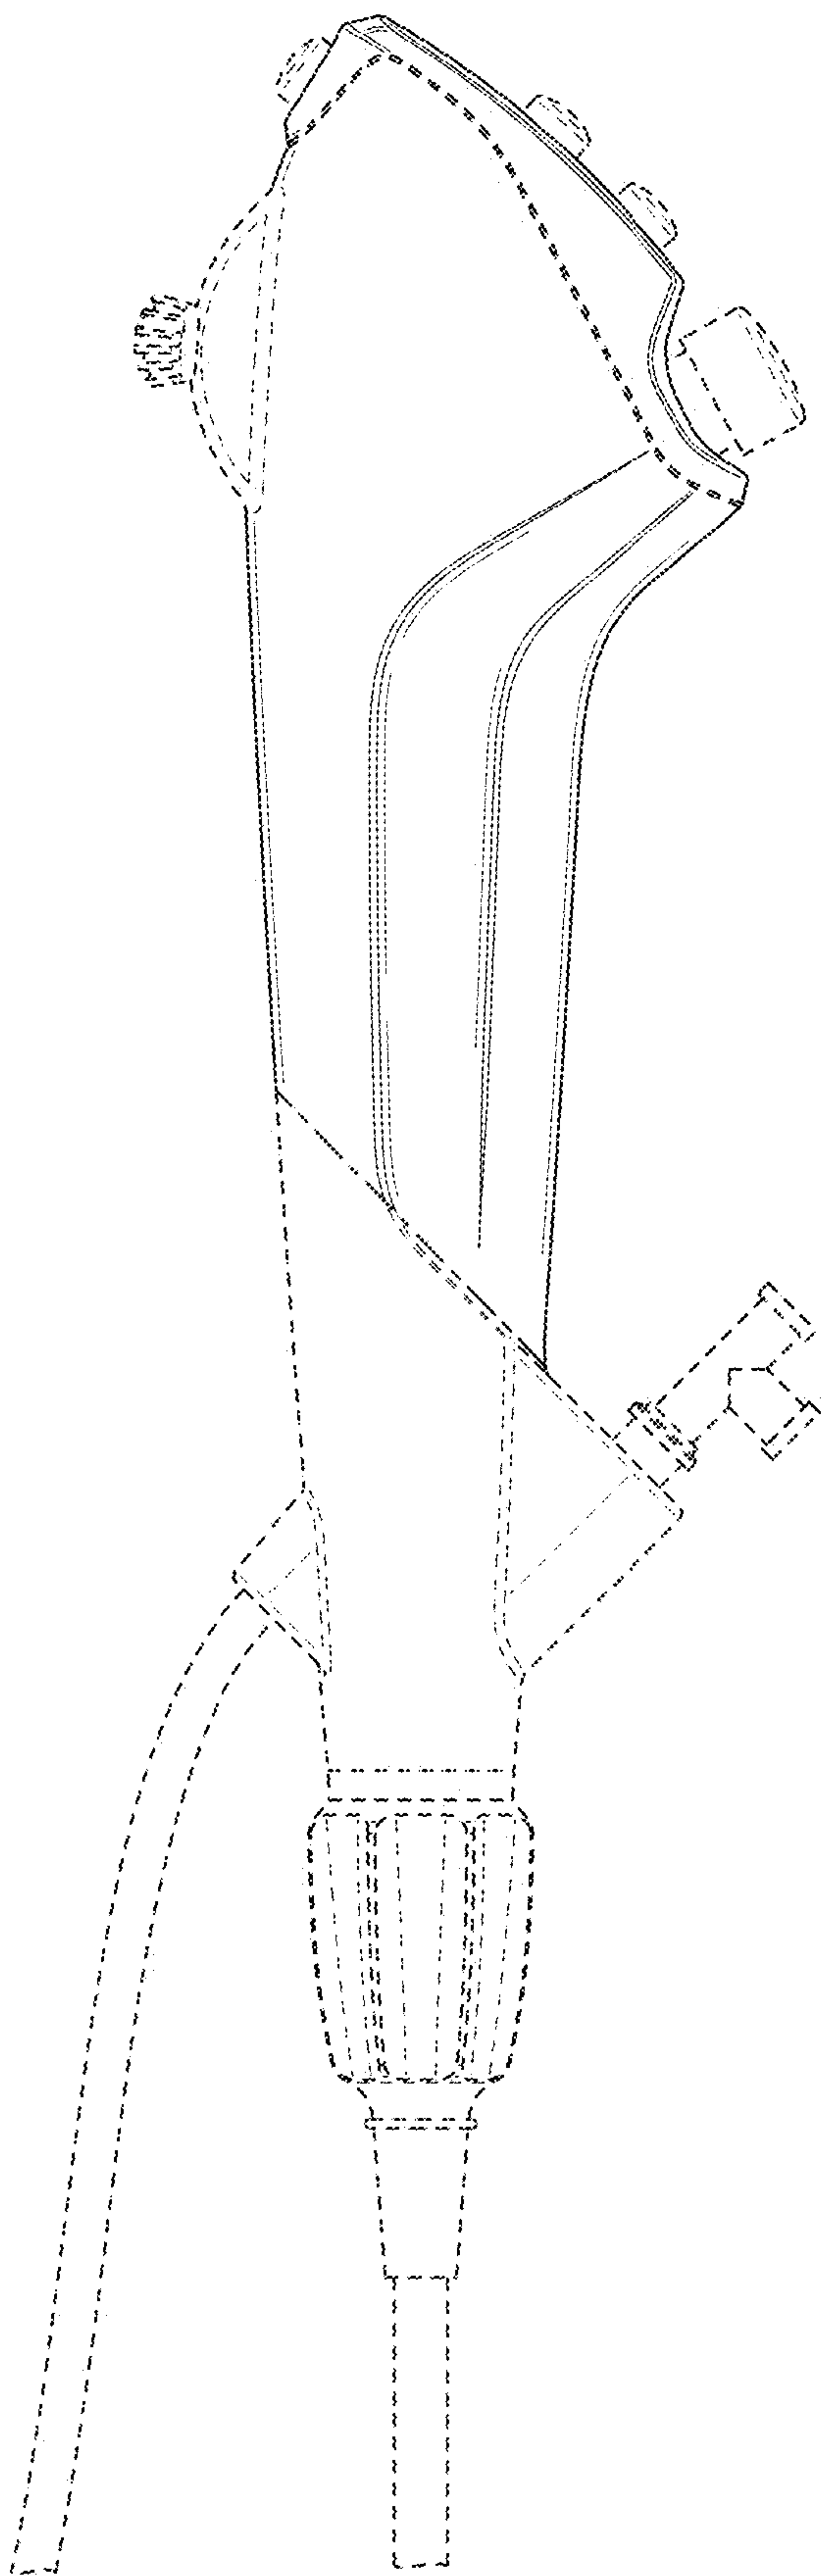


FIG. 18

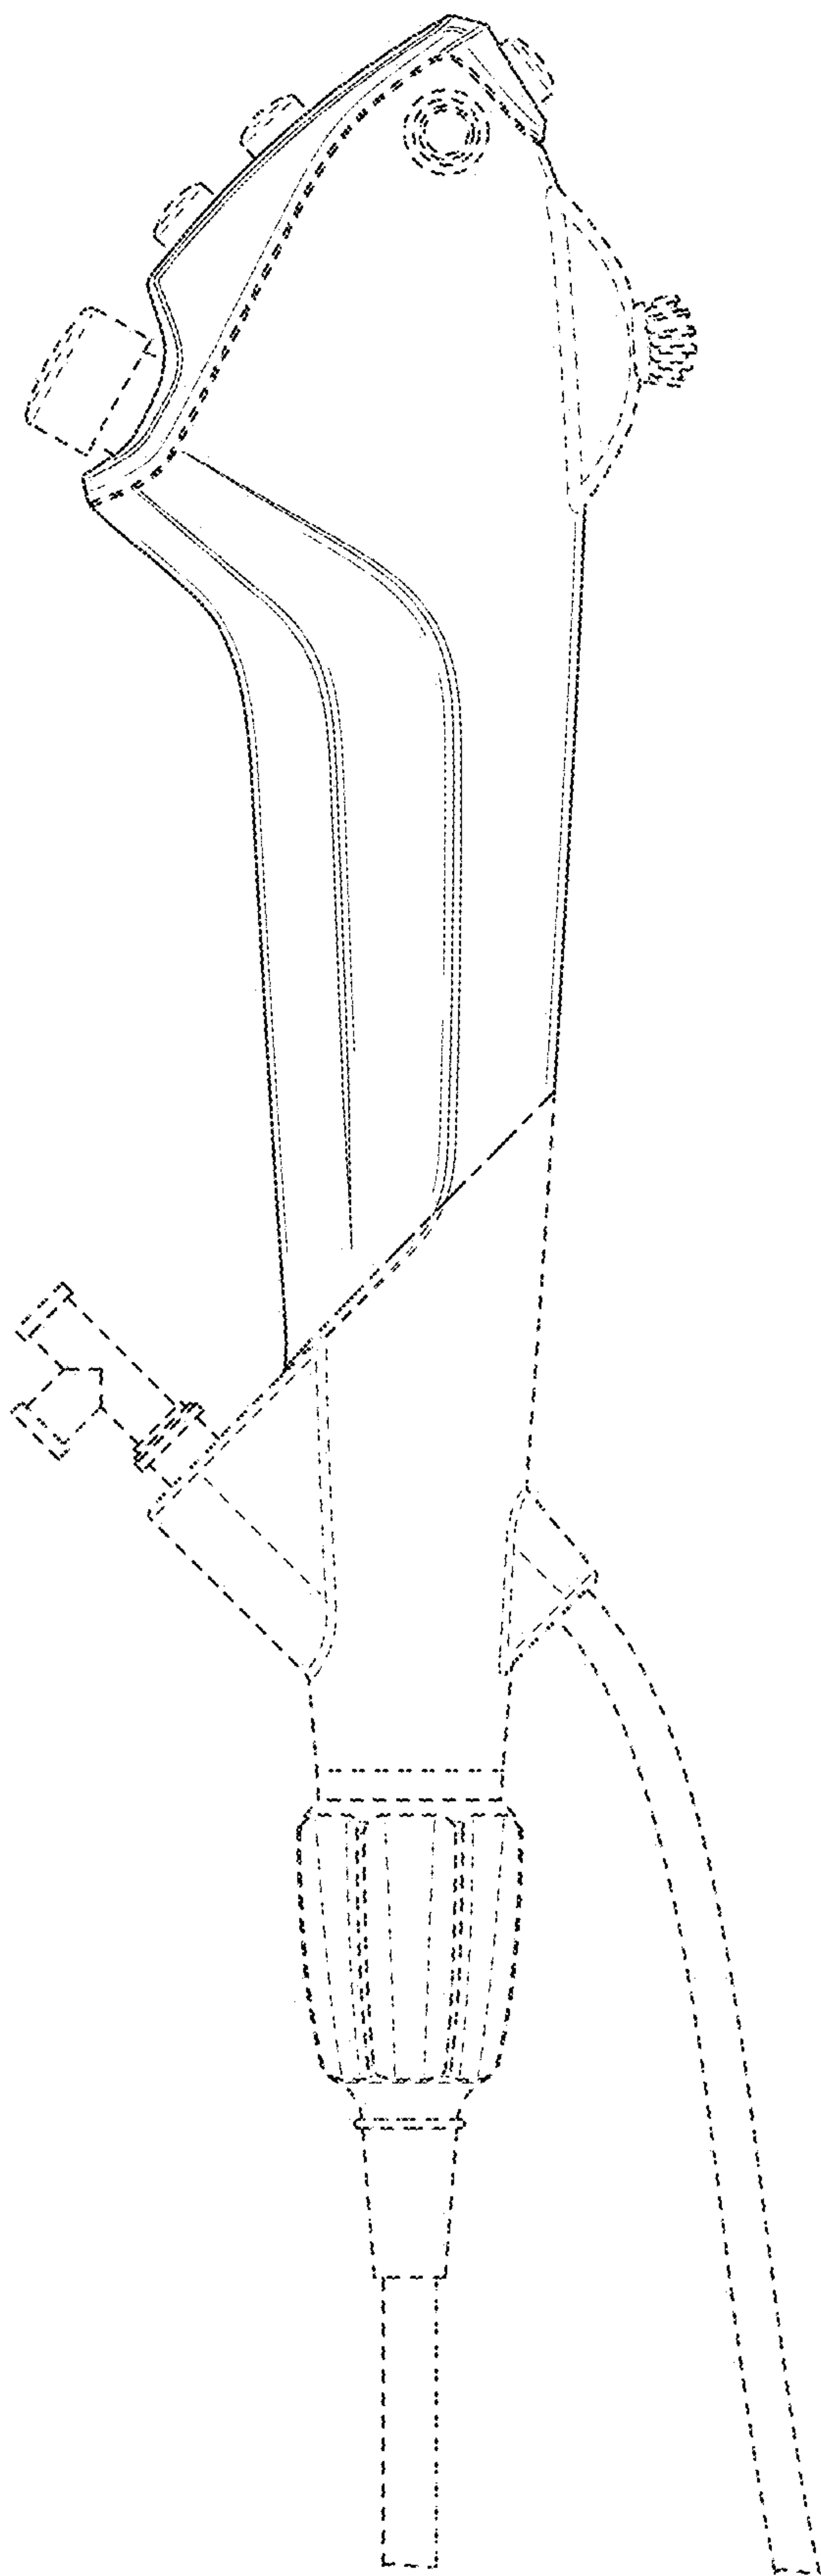


FIG. 19

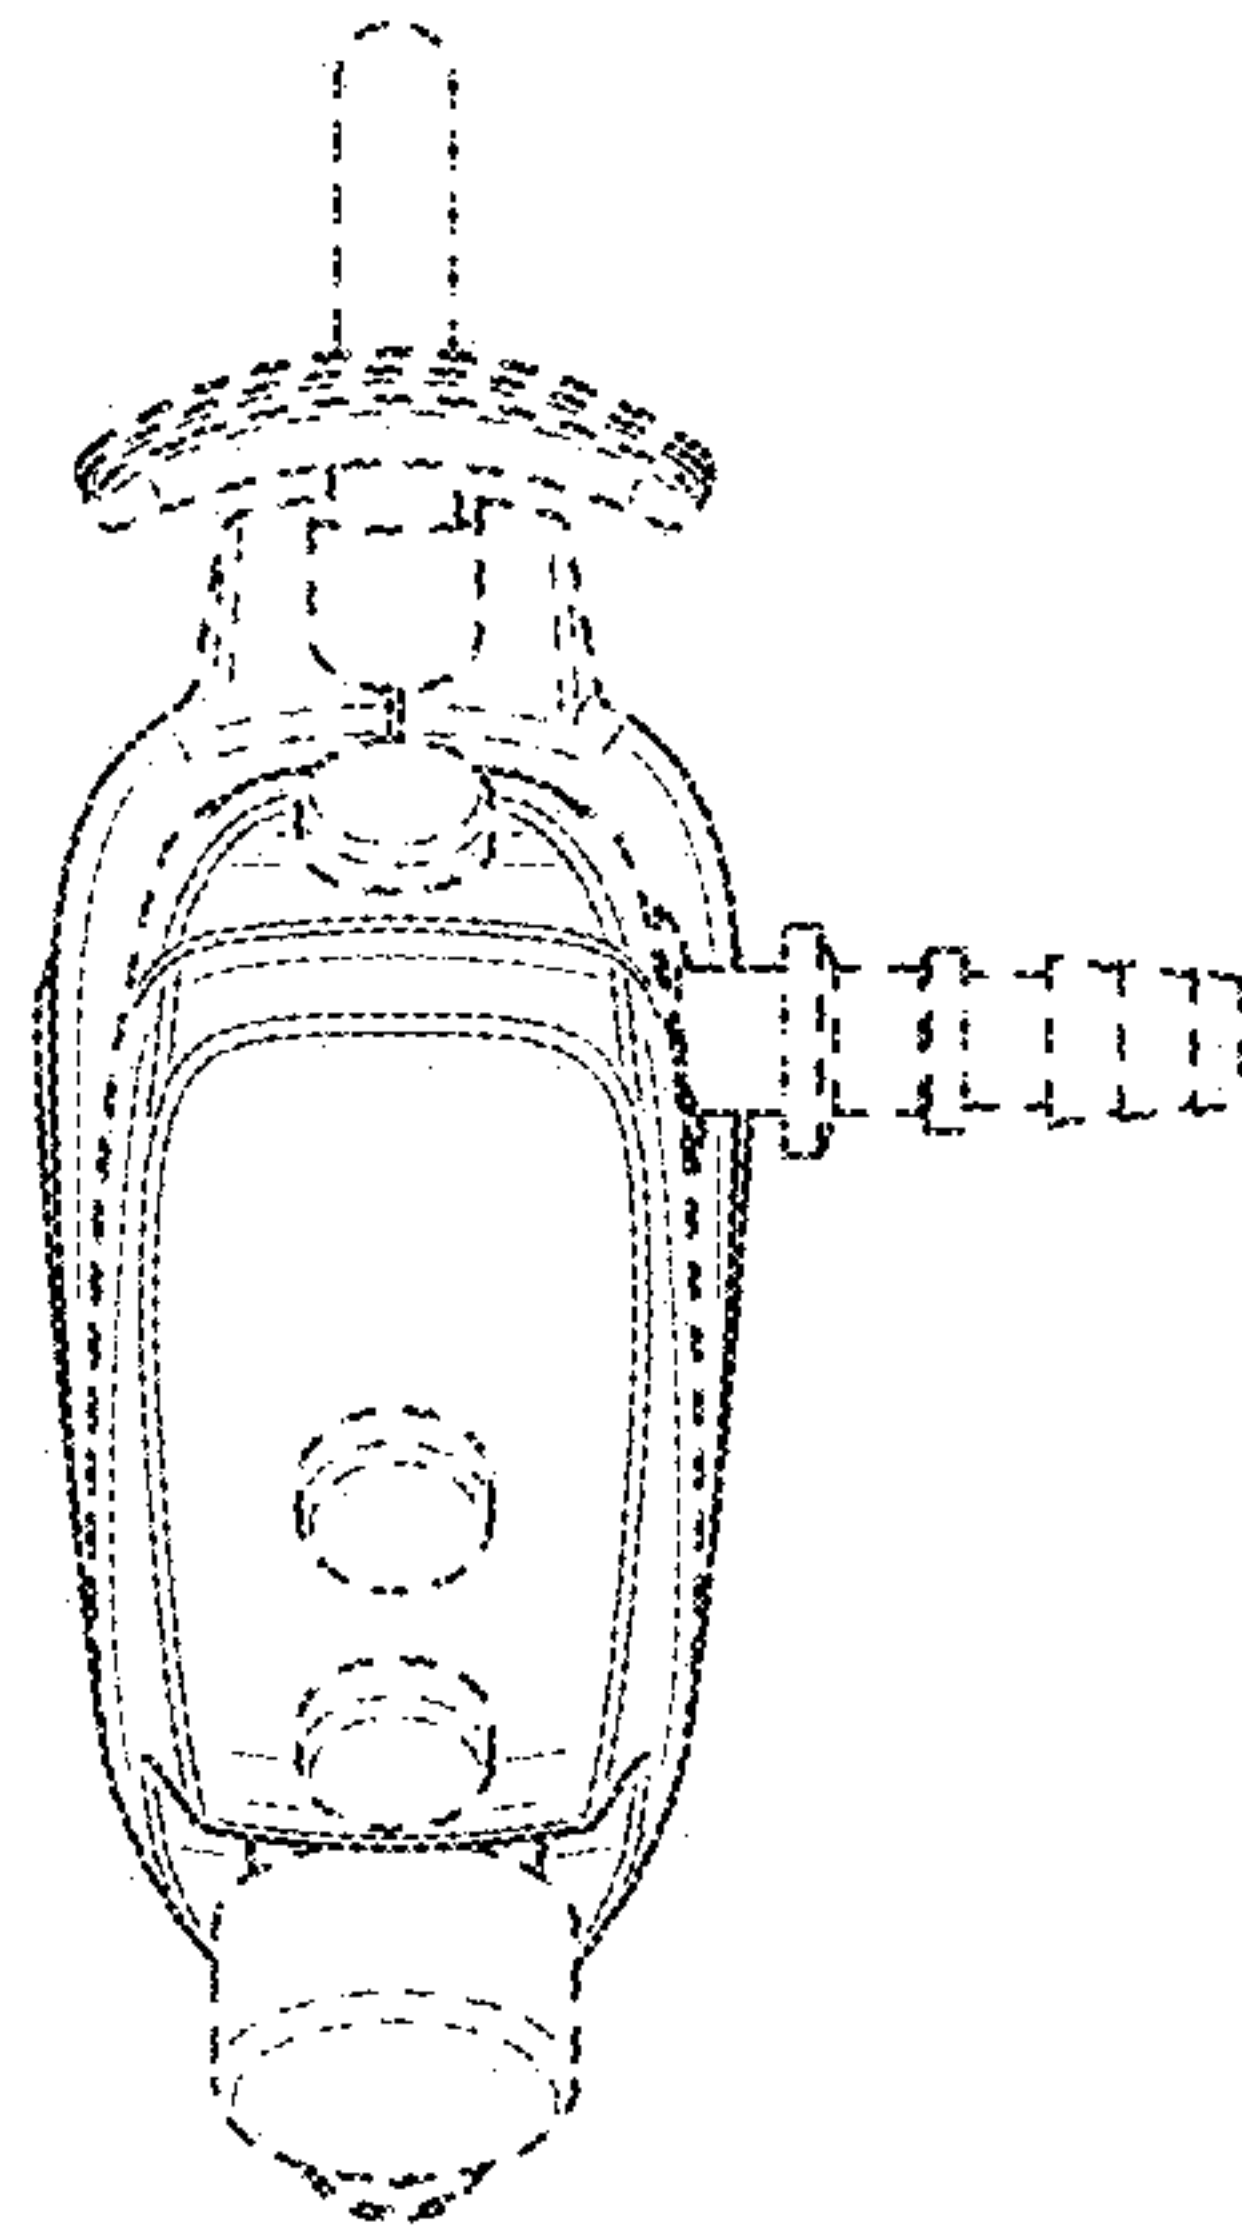


FIG. 20

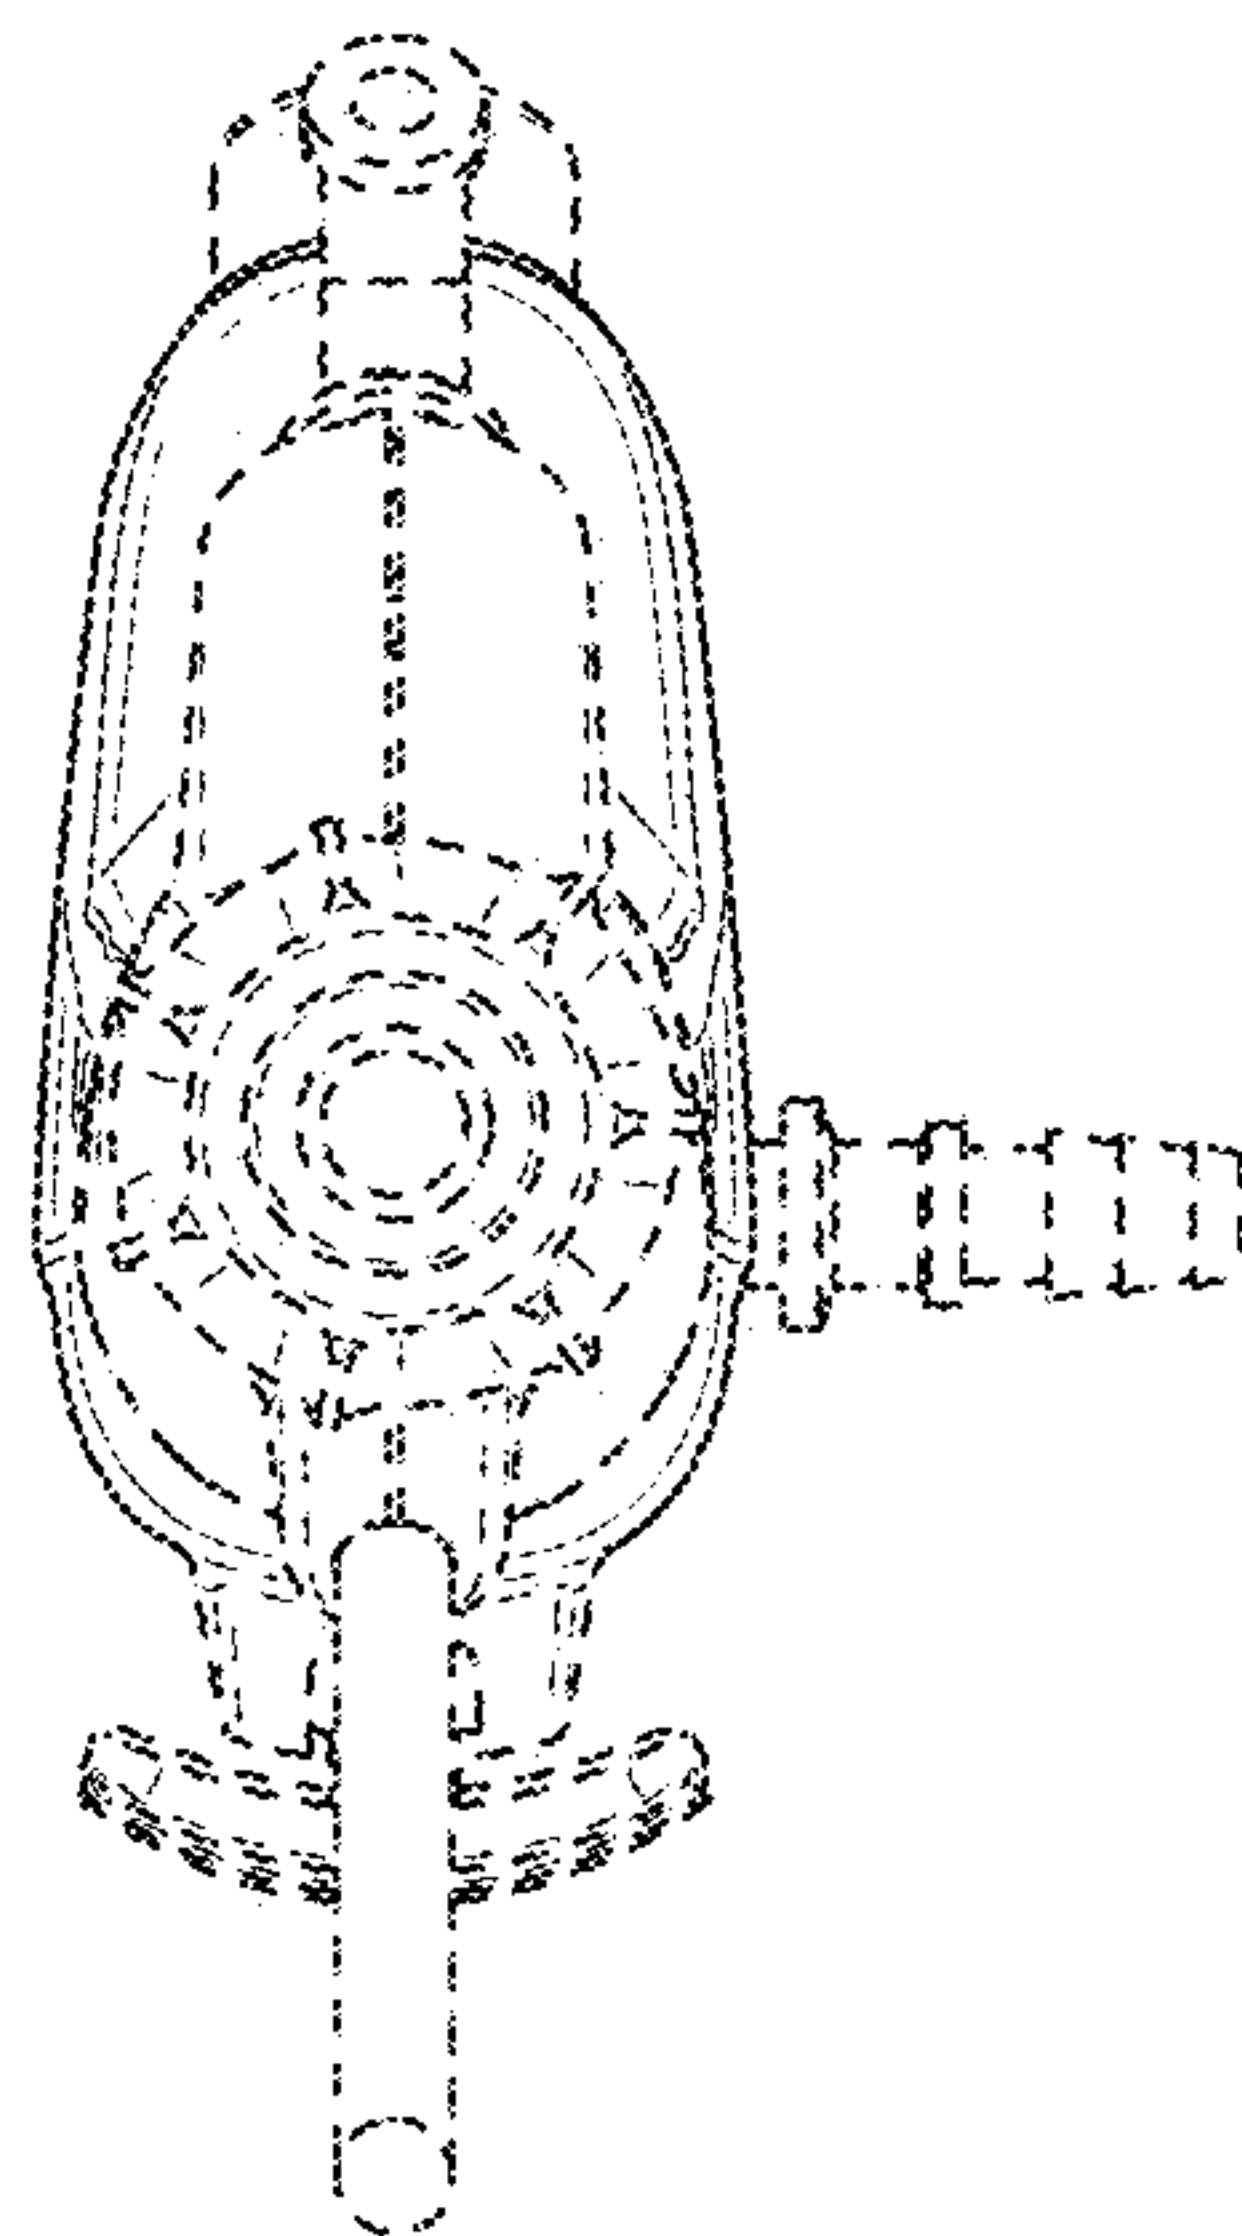


FIG. 21