



US0D1022218S

(12)

United States Design Patent

Kelly et al.

(10)

Patent No.:

US D1,022,218 S

(45)

Date of Patent:

** Apr. 9, 2024

(54) PORTABLE DROP TREATMENT DEVICE

(71) Applicant: ChiroLux LLC, Spokane, WA (US)

(72) Inventors: Maxwell Hayes Kelly, Spokane, WA (US); Jason Josiah Kiu, Spokane, WA (US)

(73) Assignee: ChiroLux LLC, Spokane, WA (US)

(**) Term: 15 Years

(21) Appl. No.: 29/808,912

(22) Filed: Sep. 23, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/183

(58) Field of Classification Search
USPC D24/159, 183–184, 200, 171; D21/671, D21/673, 675, 676, 686, 687, 690; D6/349, 360, 364, 369, 429, 595–596, D6/601, 604, 605, 610, 716.2, 718, 718.3
CPC A61G 7/00; A61G 7/0507; A61G 13/107; A47C 7/54
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D202,250	S	*	9/1965	Hauser	D6/406.3
D341,053	S	*	11/1993	Hassel	D6/601
D399,970	S	*	10/1998	Agarwala	D24/200
D492,036	S	*	6/2004	Kang	D24/200
D504,726	S	*	5/2005	Ryan	D24/200
D540,950	S	*	4/2007	Johnson	D24/183
D628,305	S	*	11/2010	Gorrec	D24/229
D718,456	S	*	11/2014	McNamee	D24/171

D736,867	S	*	8/2015	Glickfield	D21/671
D880,707	S	*	4/2020	Gu	D24/200
D935,805	S	*	11/2021	Zhou	D6/601
D971,587	S	*	12/2022	Bronkhorst	D3/203.1

OTHER PUBLICATIONS

ChiroLux Spark | 360° Extremity Portable Drop Piece Chiropractic Tool Is A Chiropractic Adjusting Tool For Adjusting Feet, Ankles, Knees, Shoulders & Wrists On Any Flat Surface. Online, published date Sep. 1, 2021. Retrieved on May 10, 2023 from URL: https://www.amazon.com/ChiroLux-Extremity-Chiropractic-Adjusting-Sho.*

* cited by examiner

Primary Examiner — Omeed Agilee

(74) Attorney, Agent, or Firm — Adibi IP Group, PC; Amir V. Adibi; Andrew C. Palmer


(57) CLAIM

The ornamental design for a portable drop treatment device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a portable drop treatment device showing our new design.
FIG. 2 is a top view thereof showing our new design.
FIG. 3 is an enlarged bottom view thereof.
FIG. 4 is a left side view thereof.
FIG. 5 is a right side view thereof.
FIG. 6 is a front view thereof; and,
FIG. 7 is a rear view thereof.
The broken lines depict portions of the portable drop treatment device that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

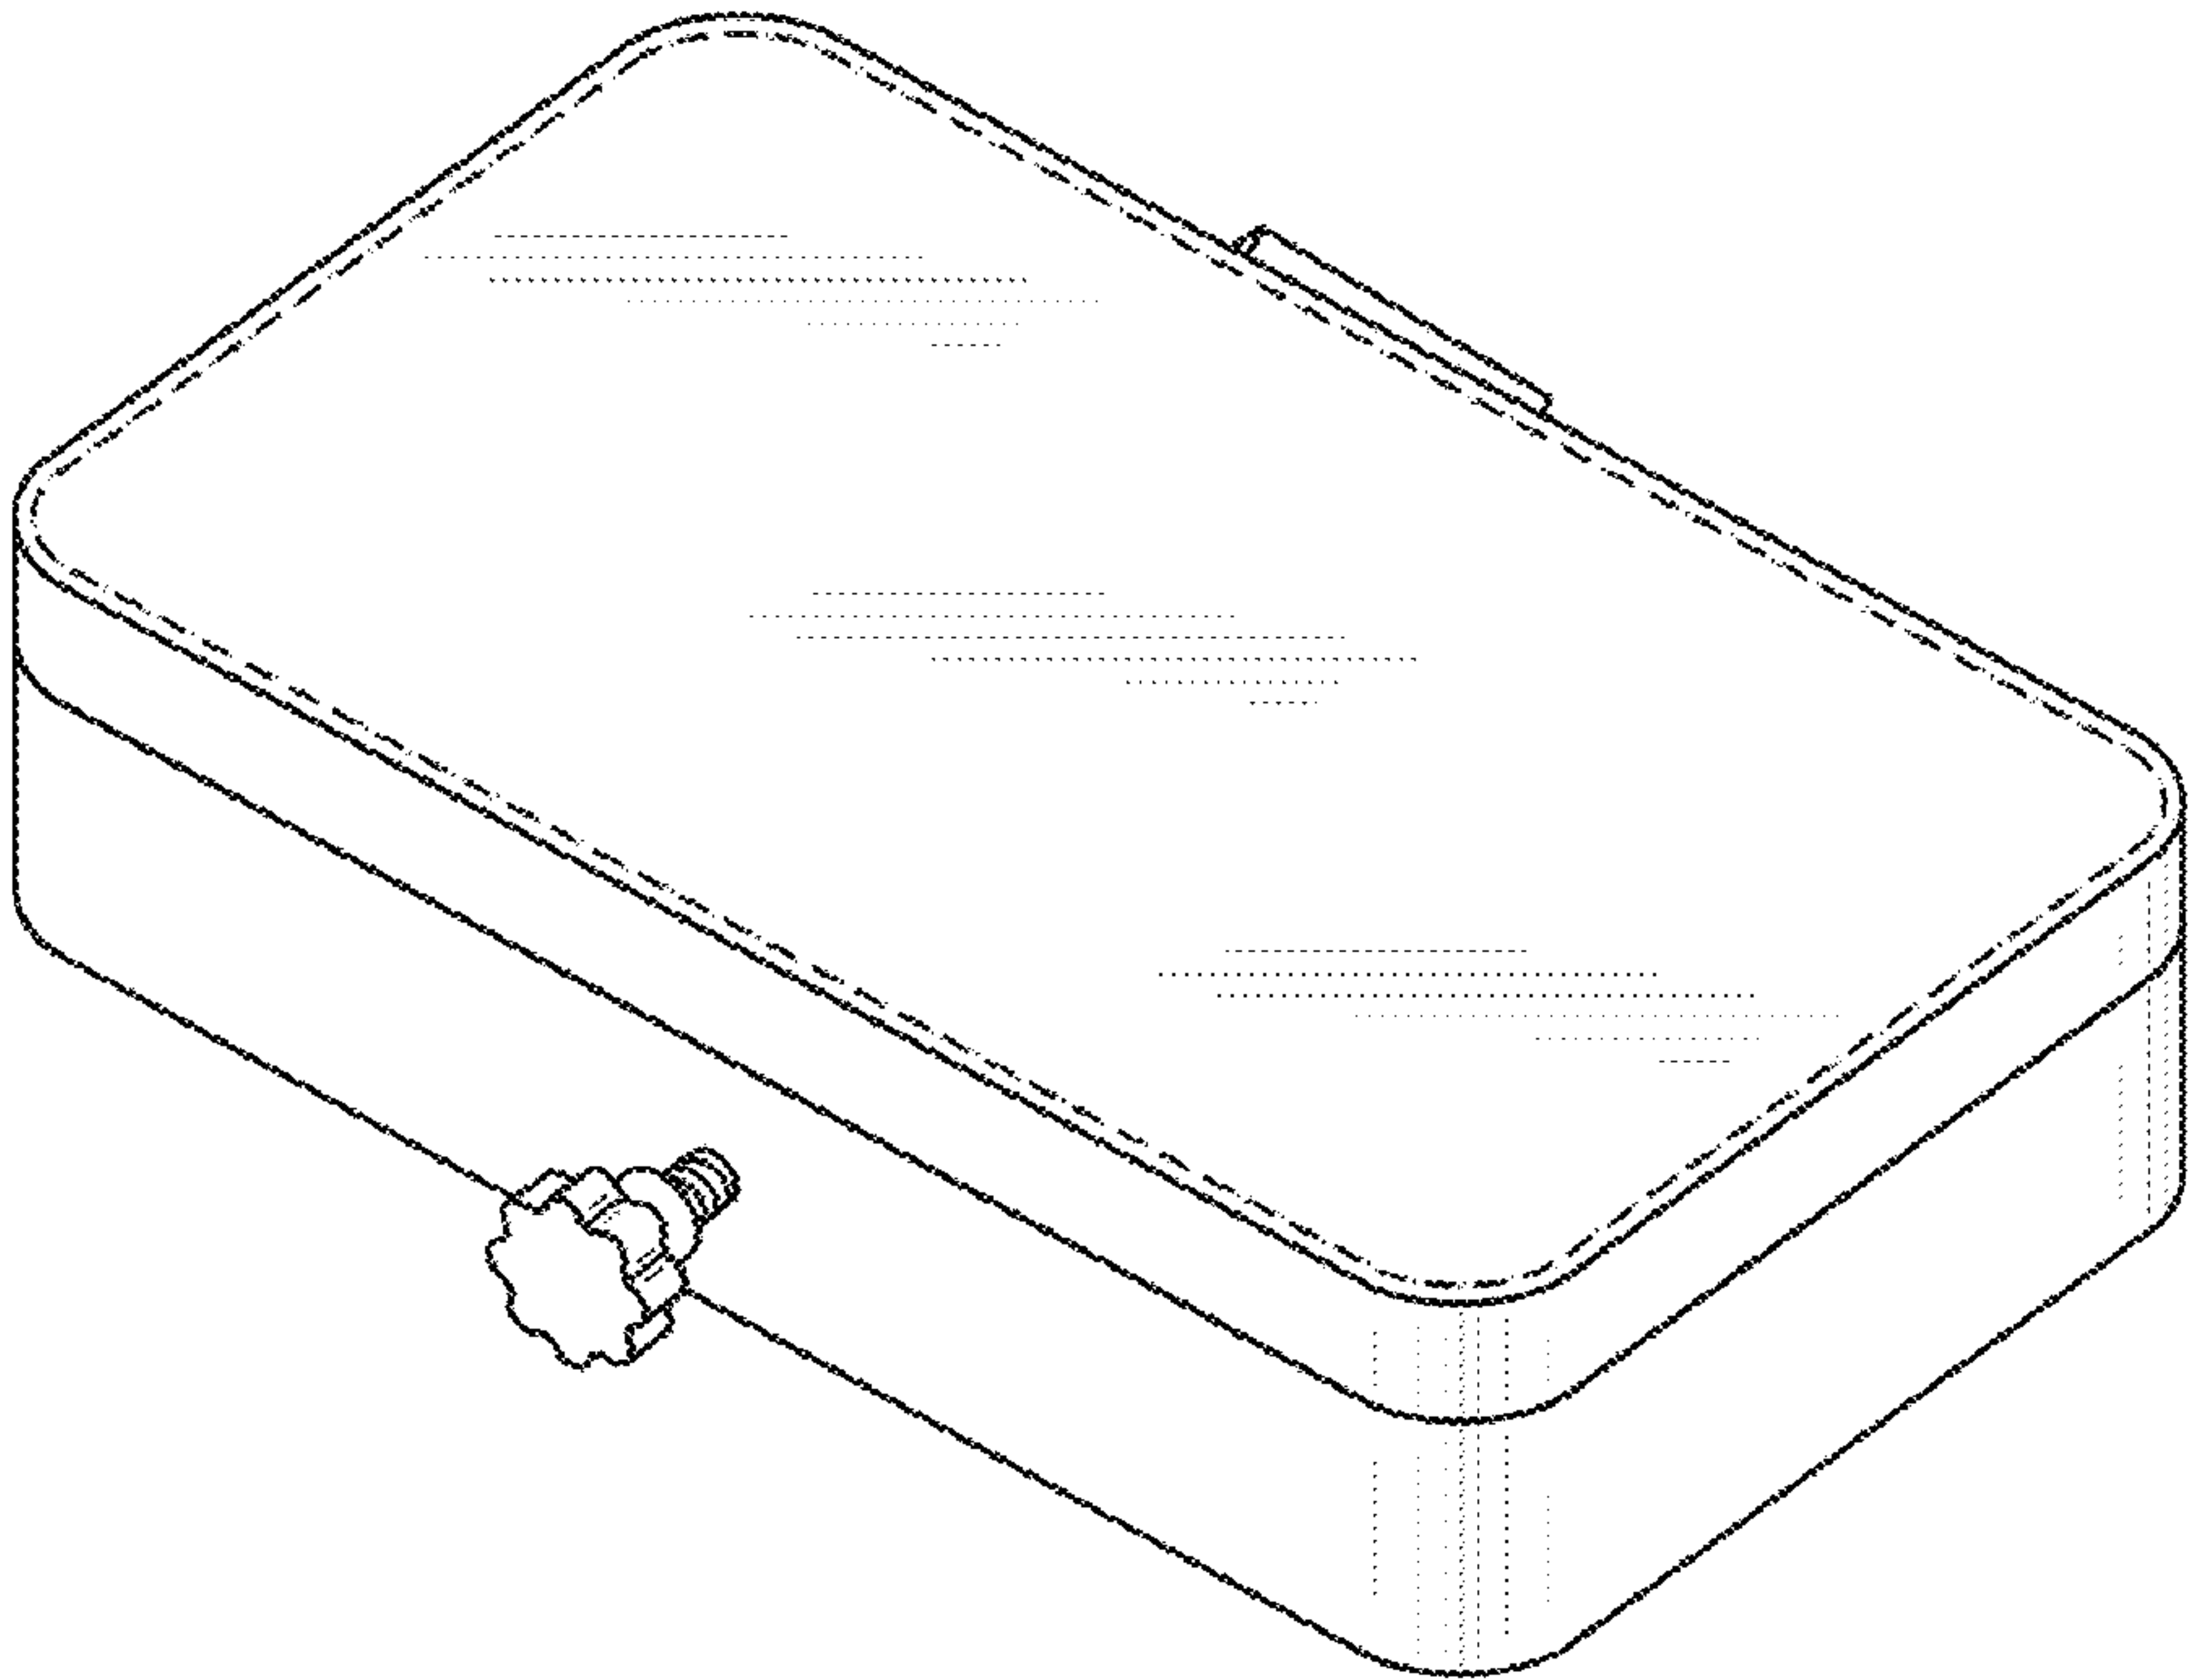

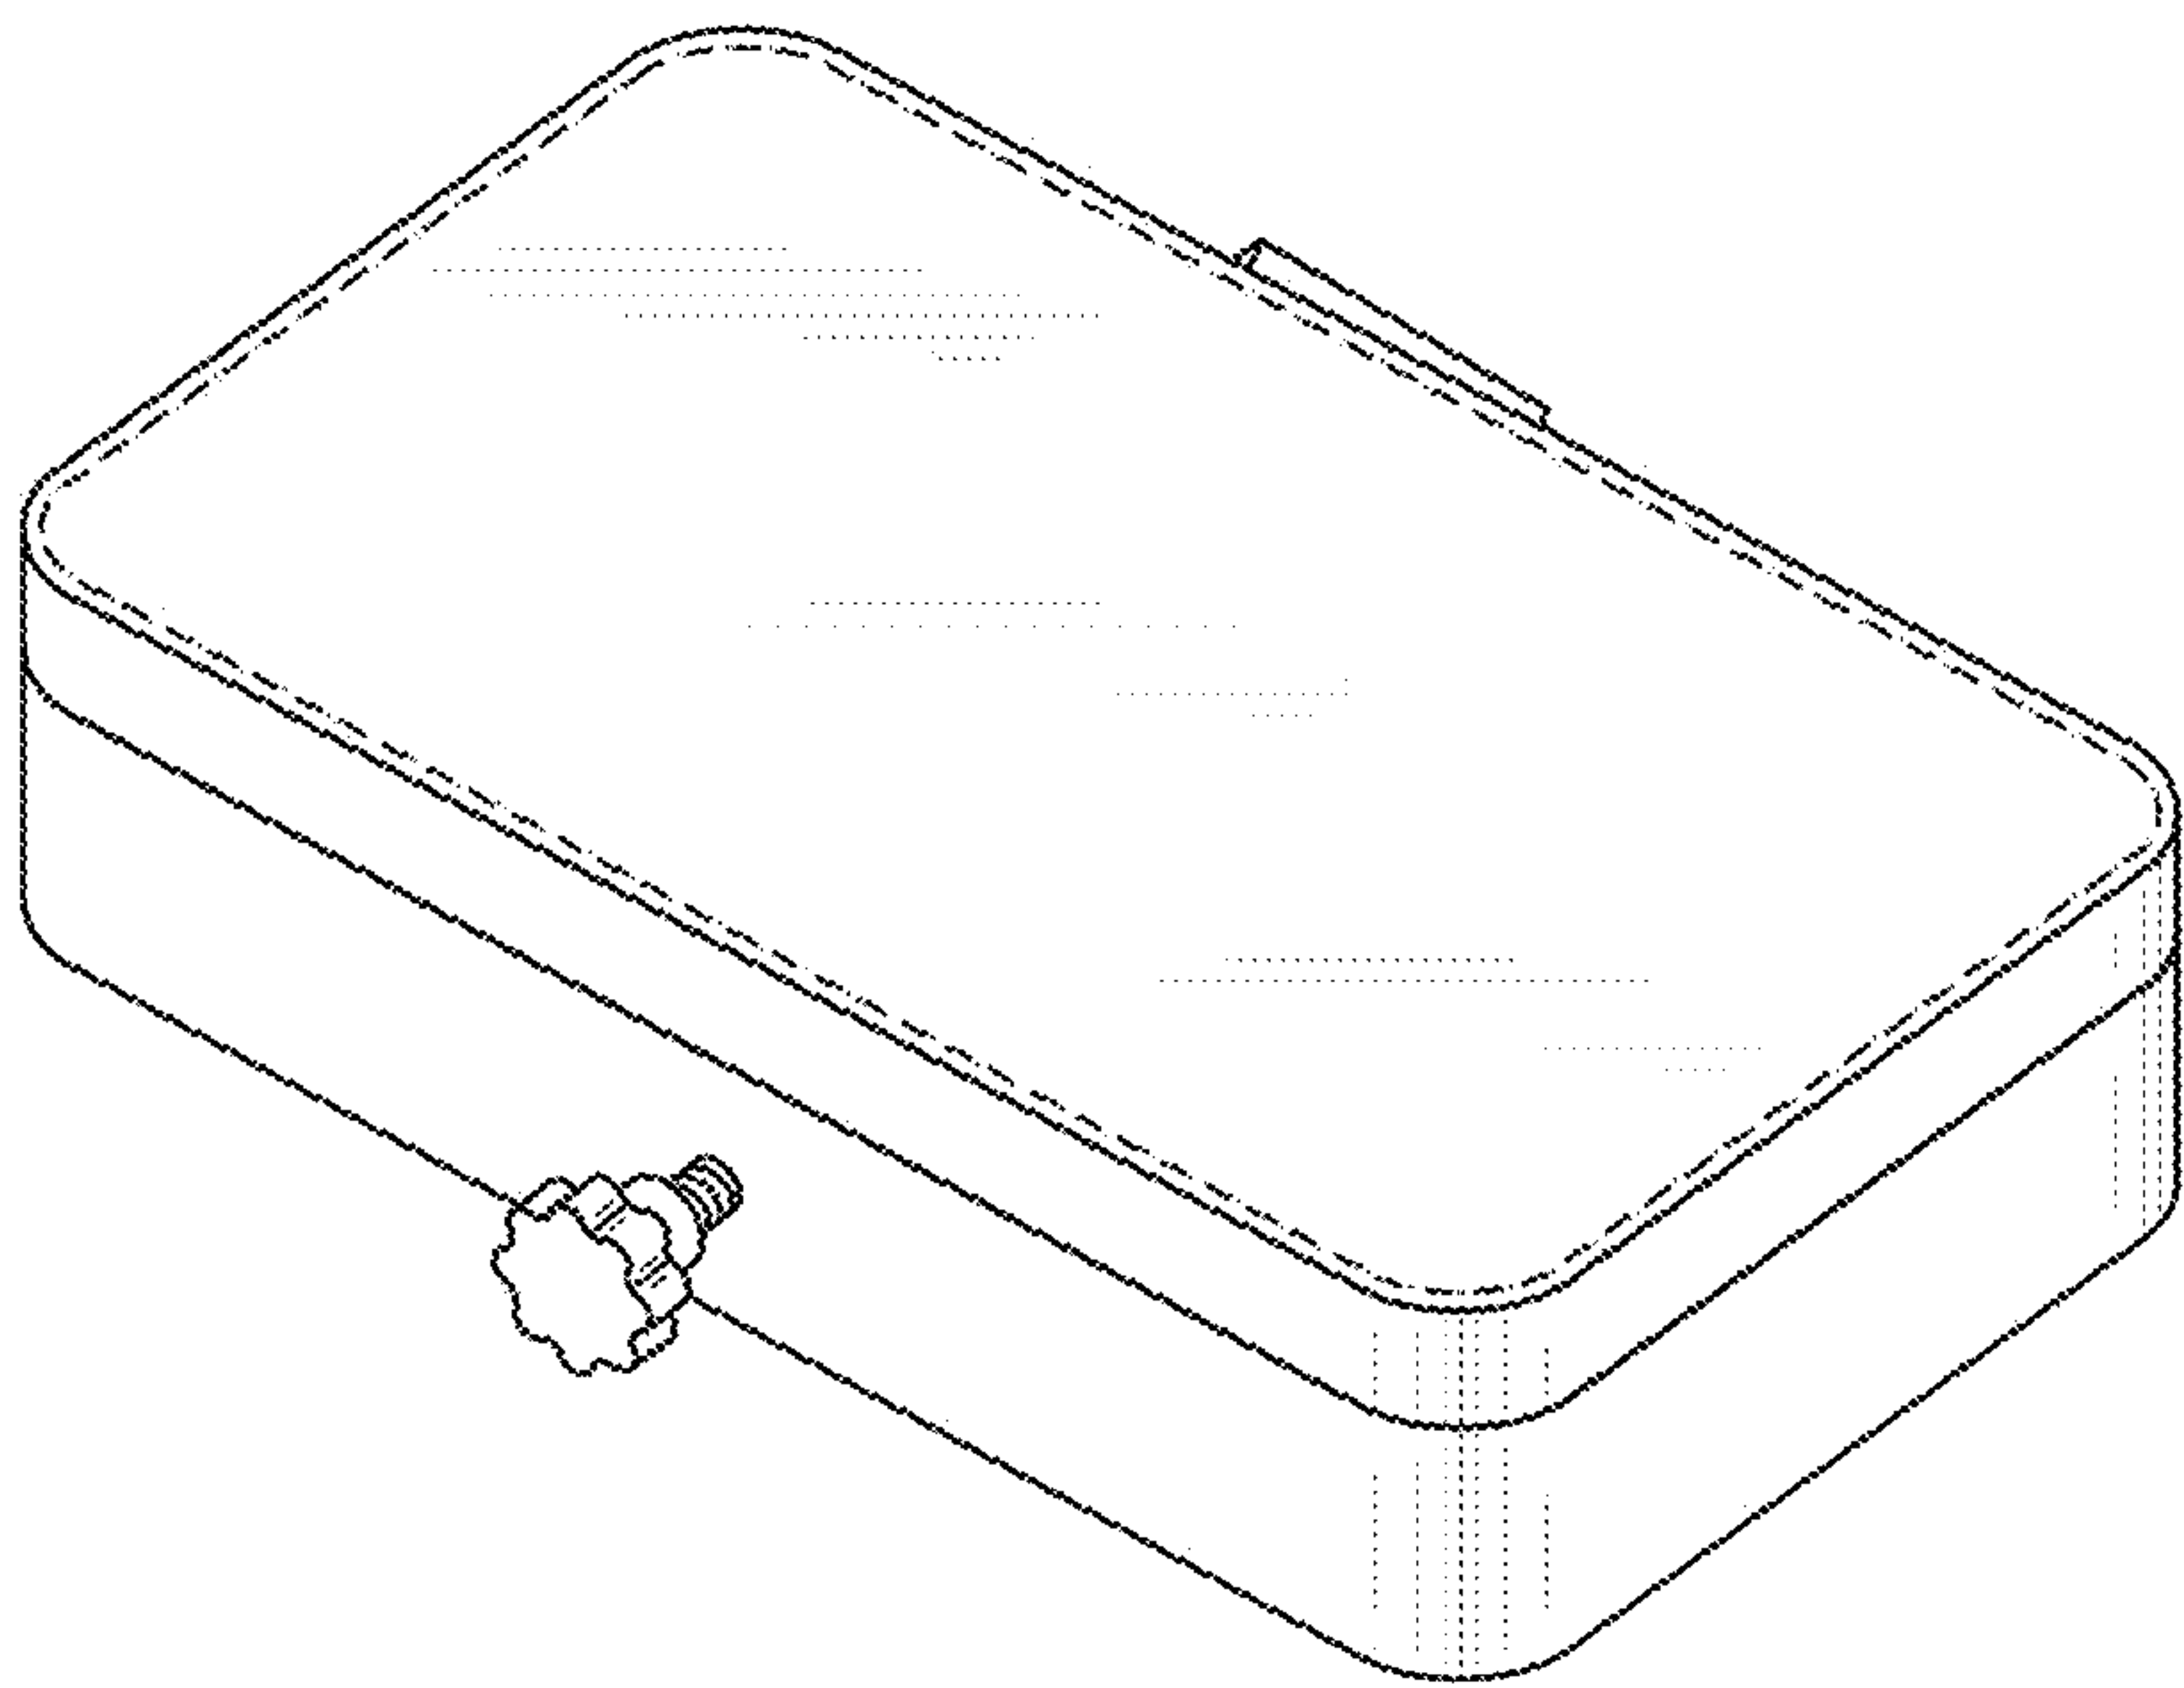


FIG. 1

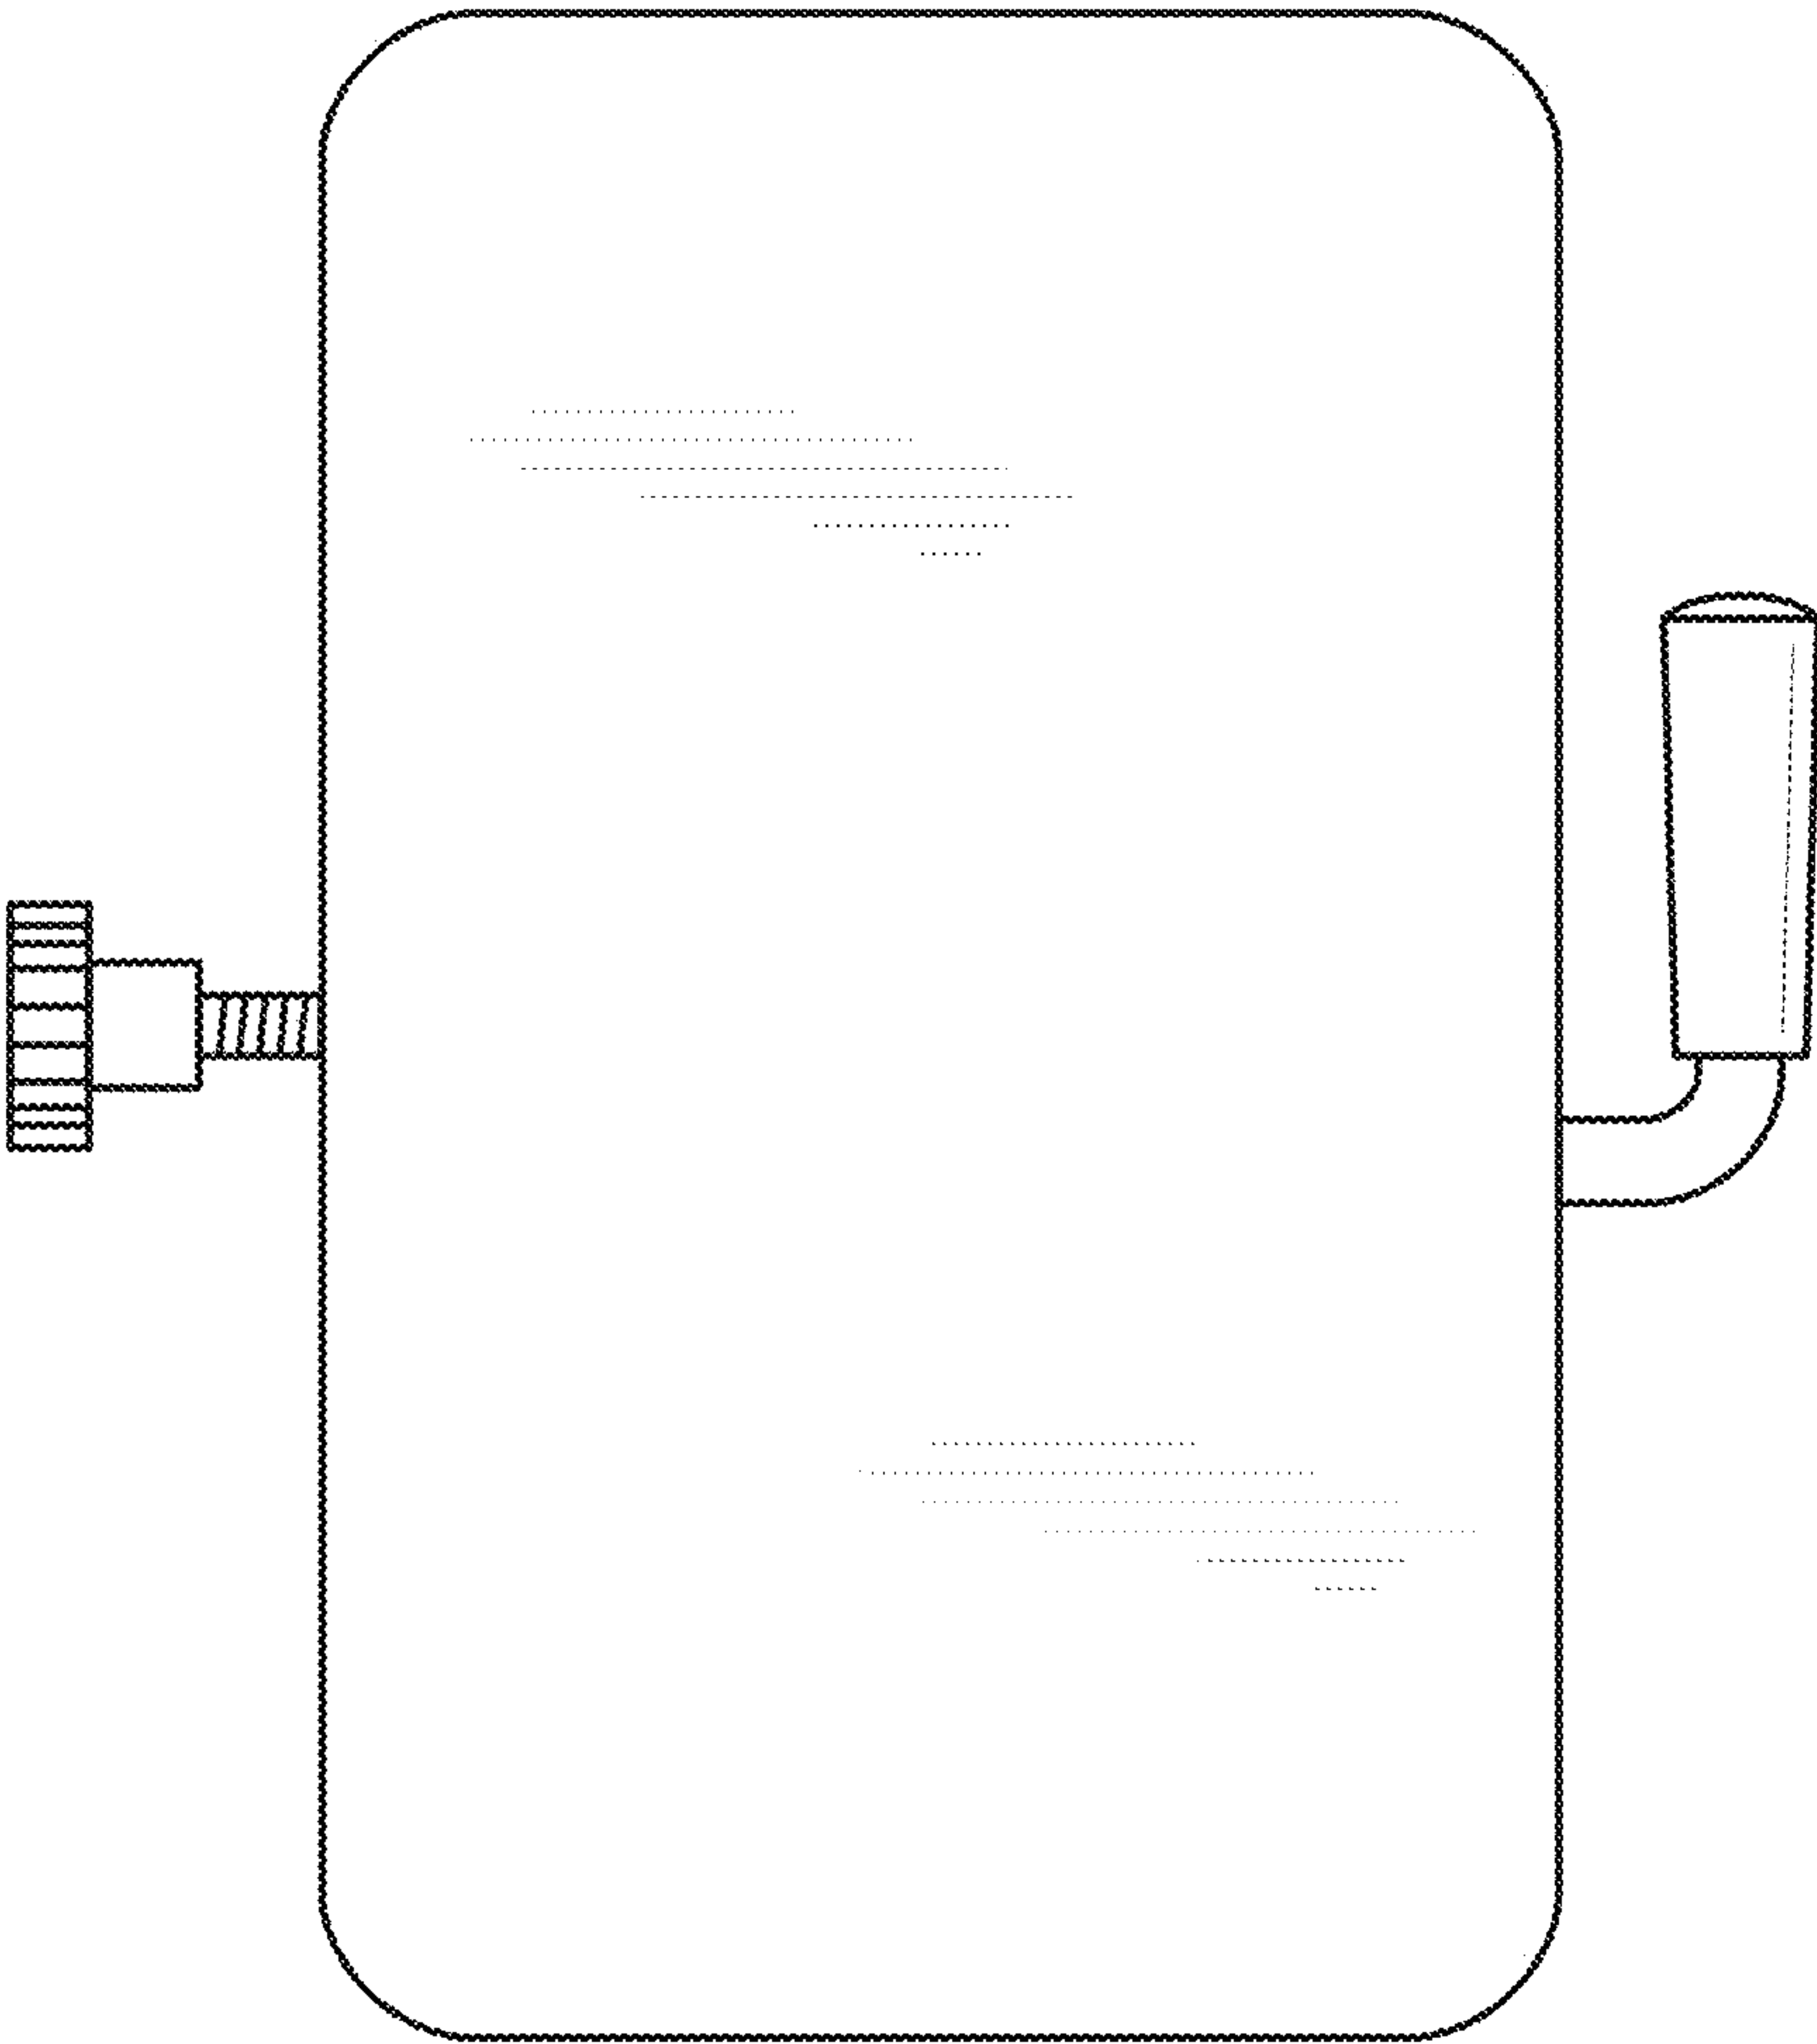


FIG. 2

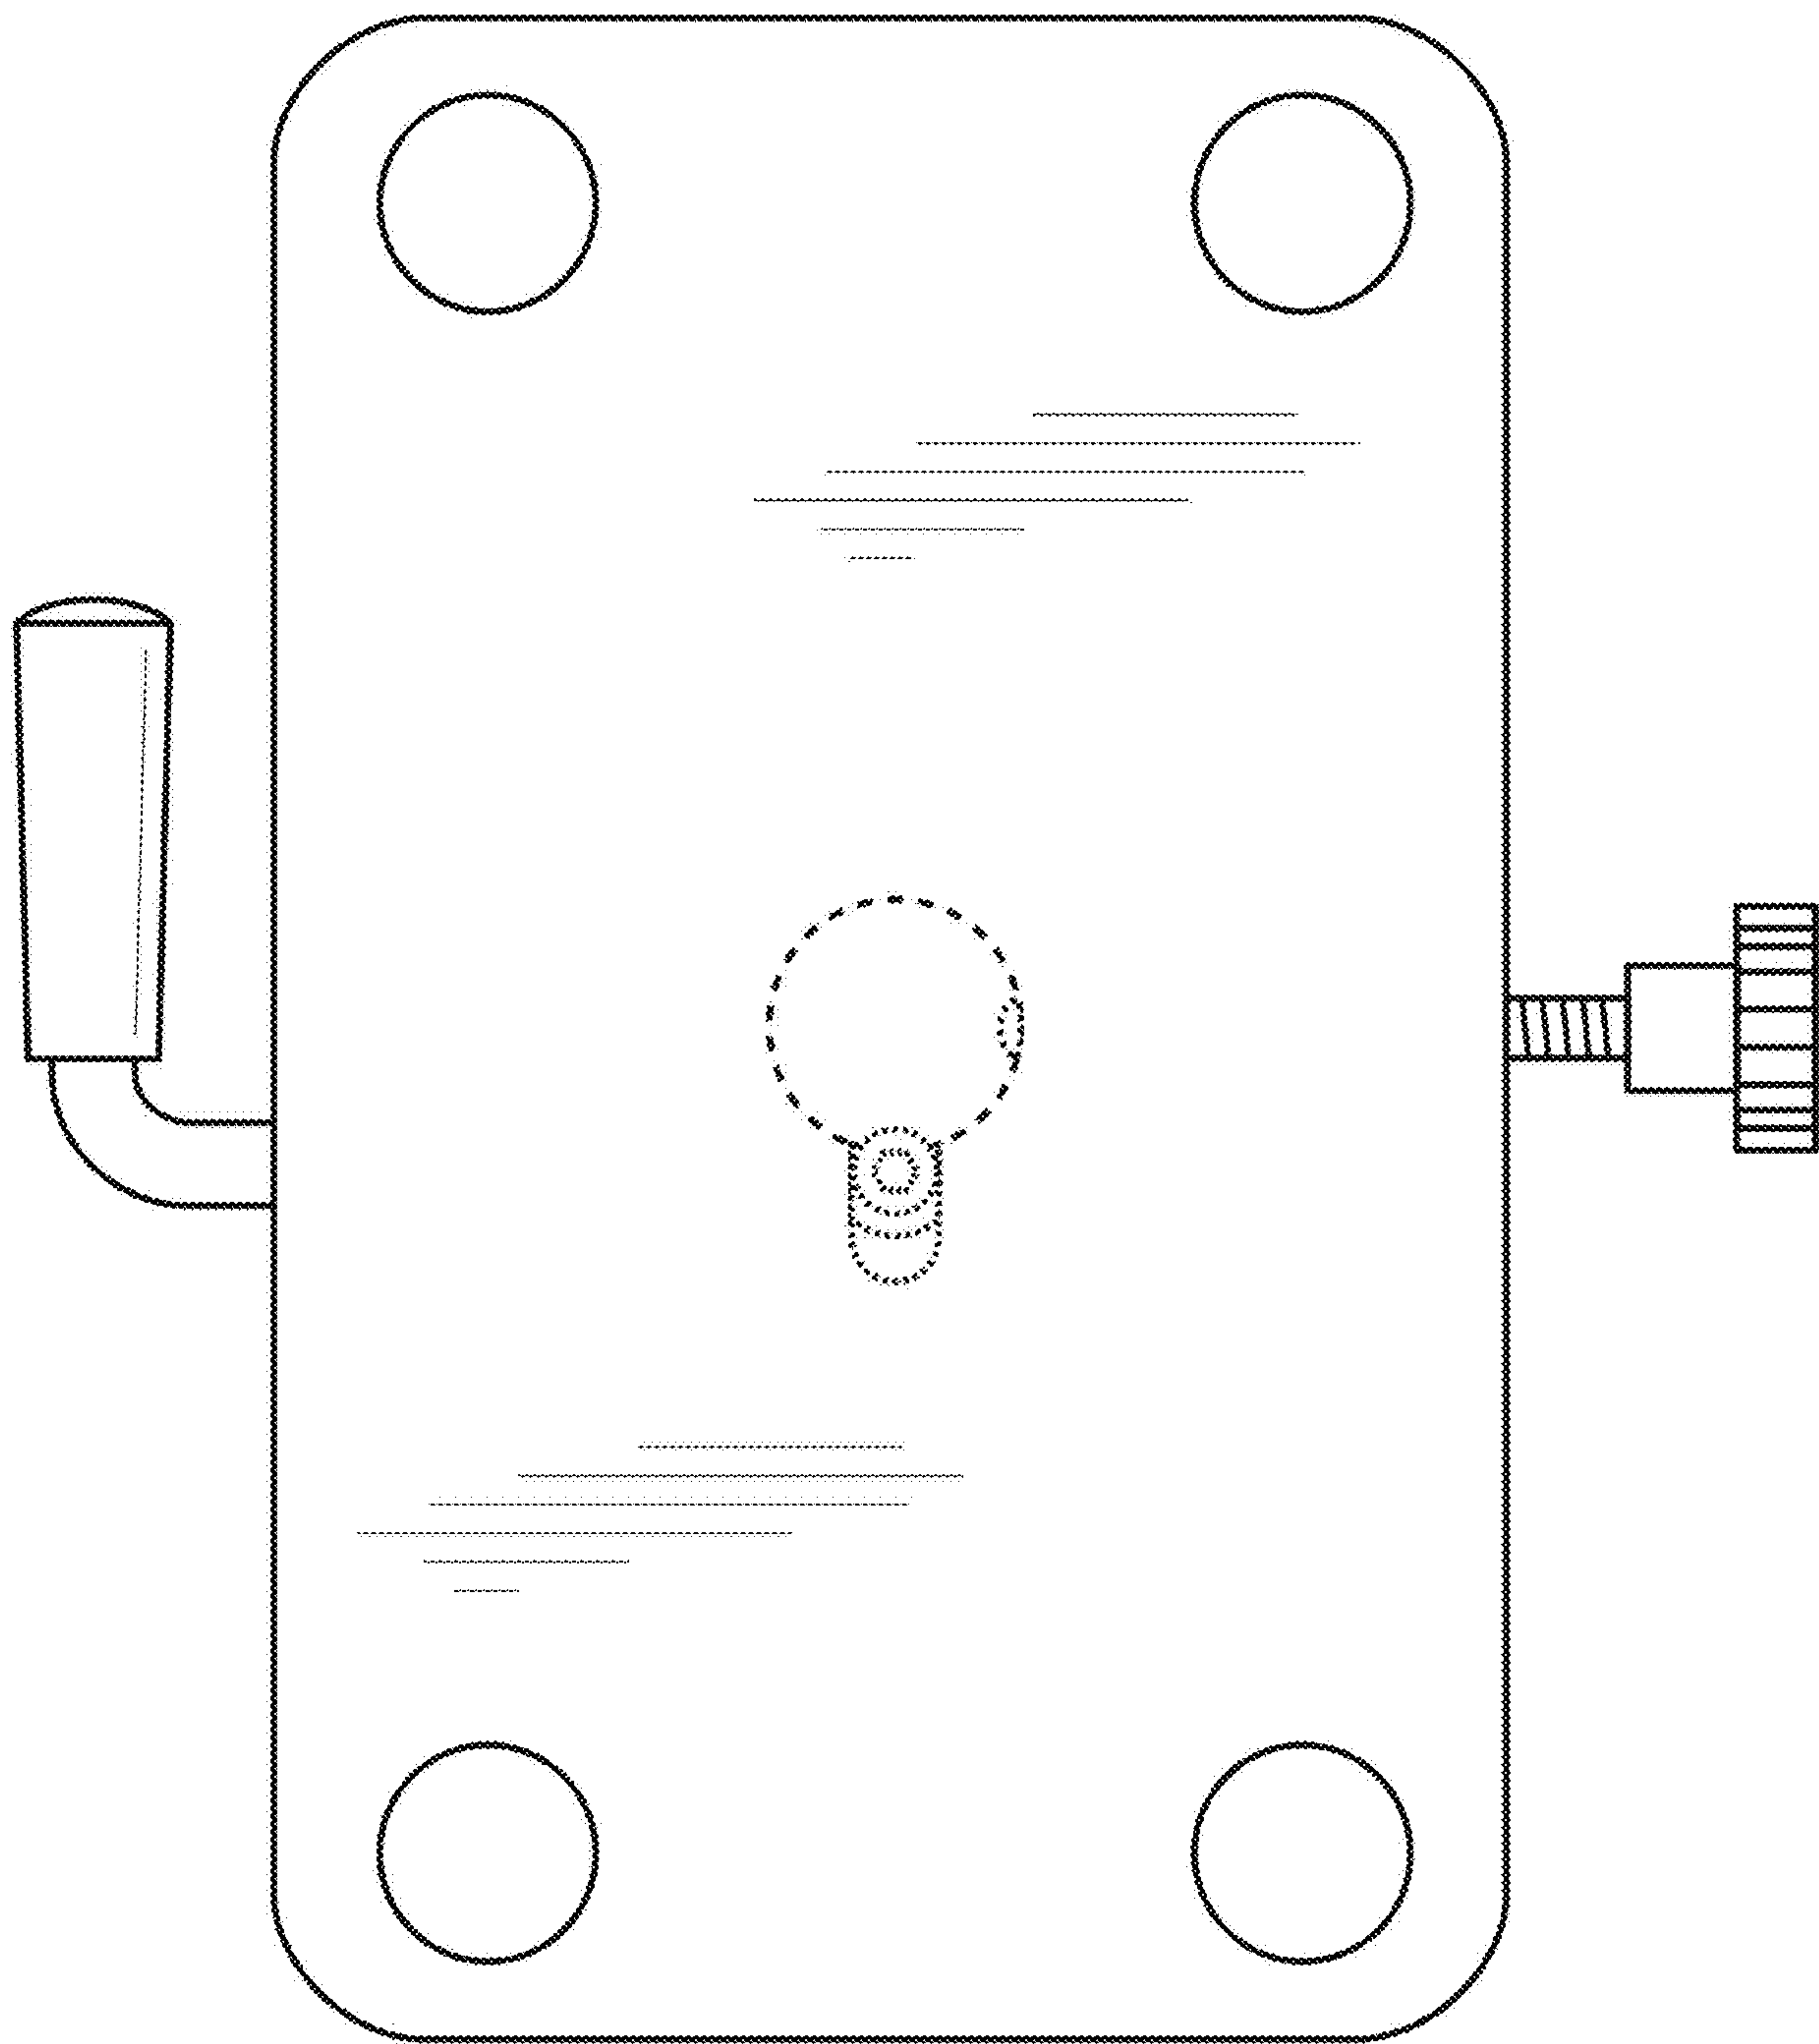


FIG. 3

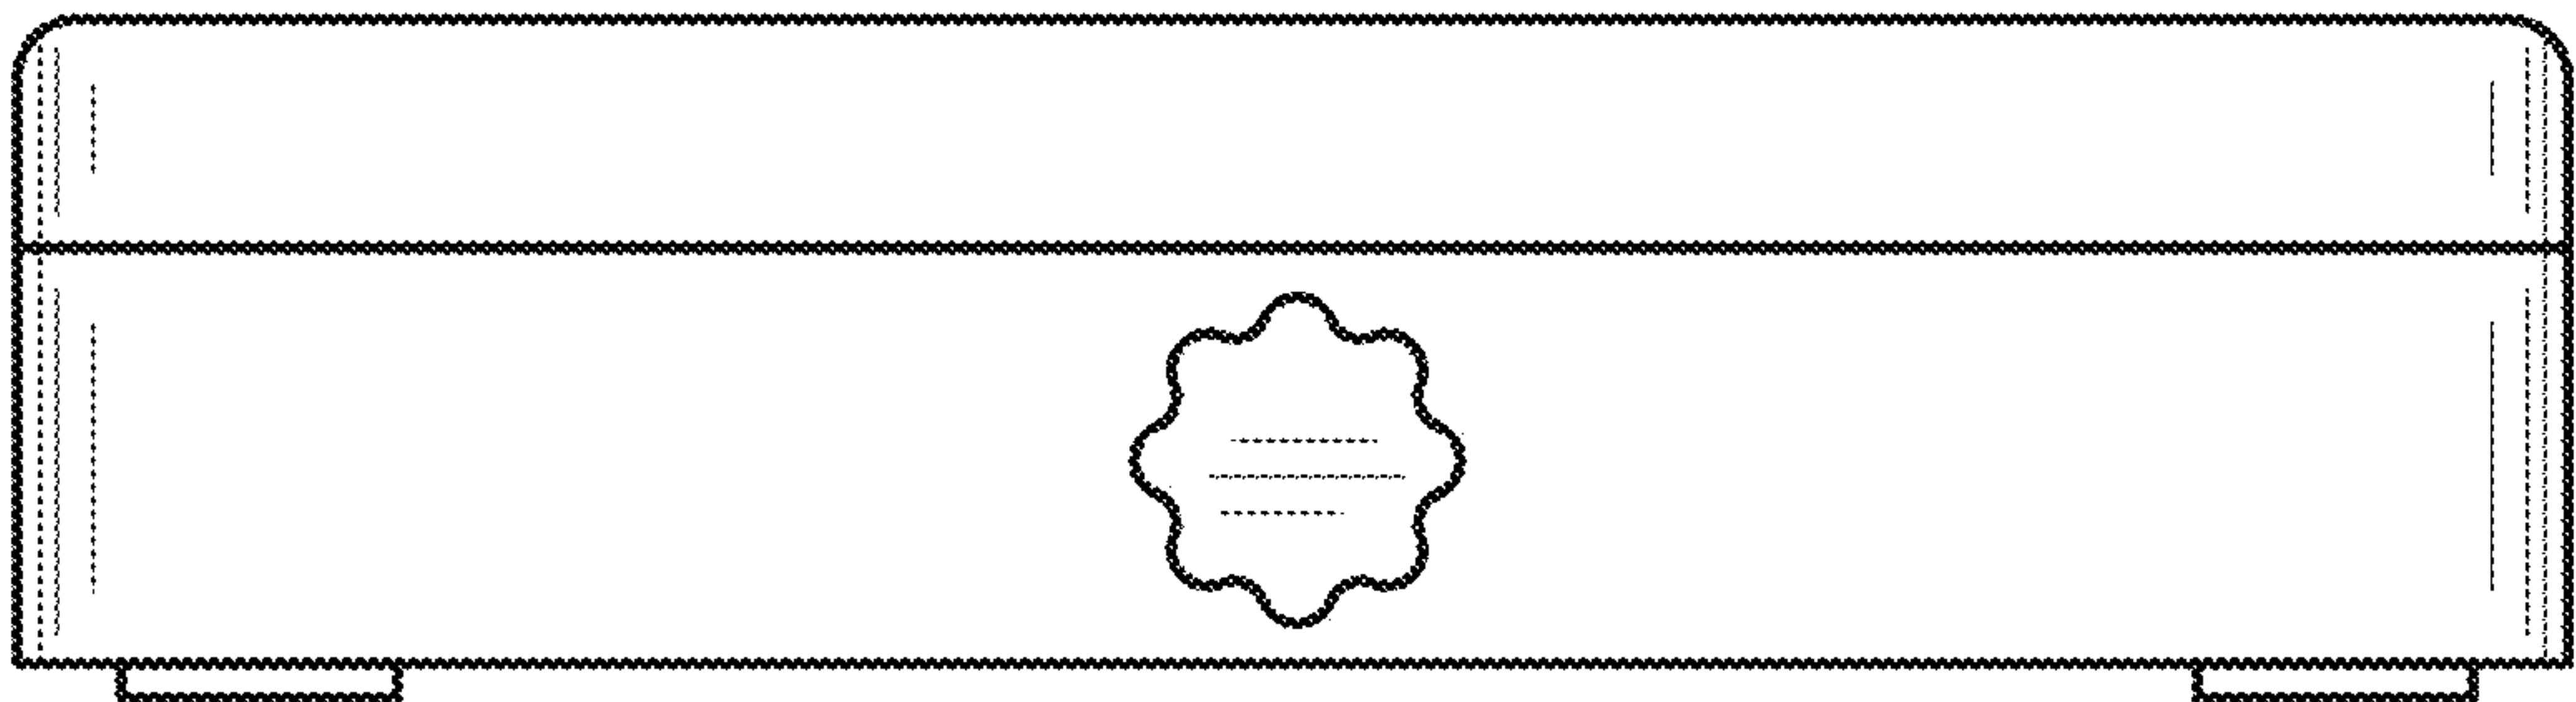


FIG. 4

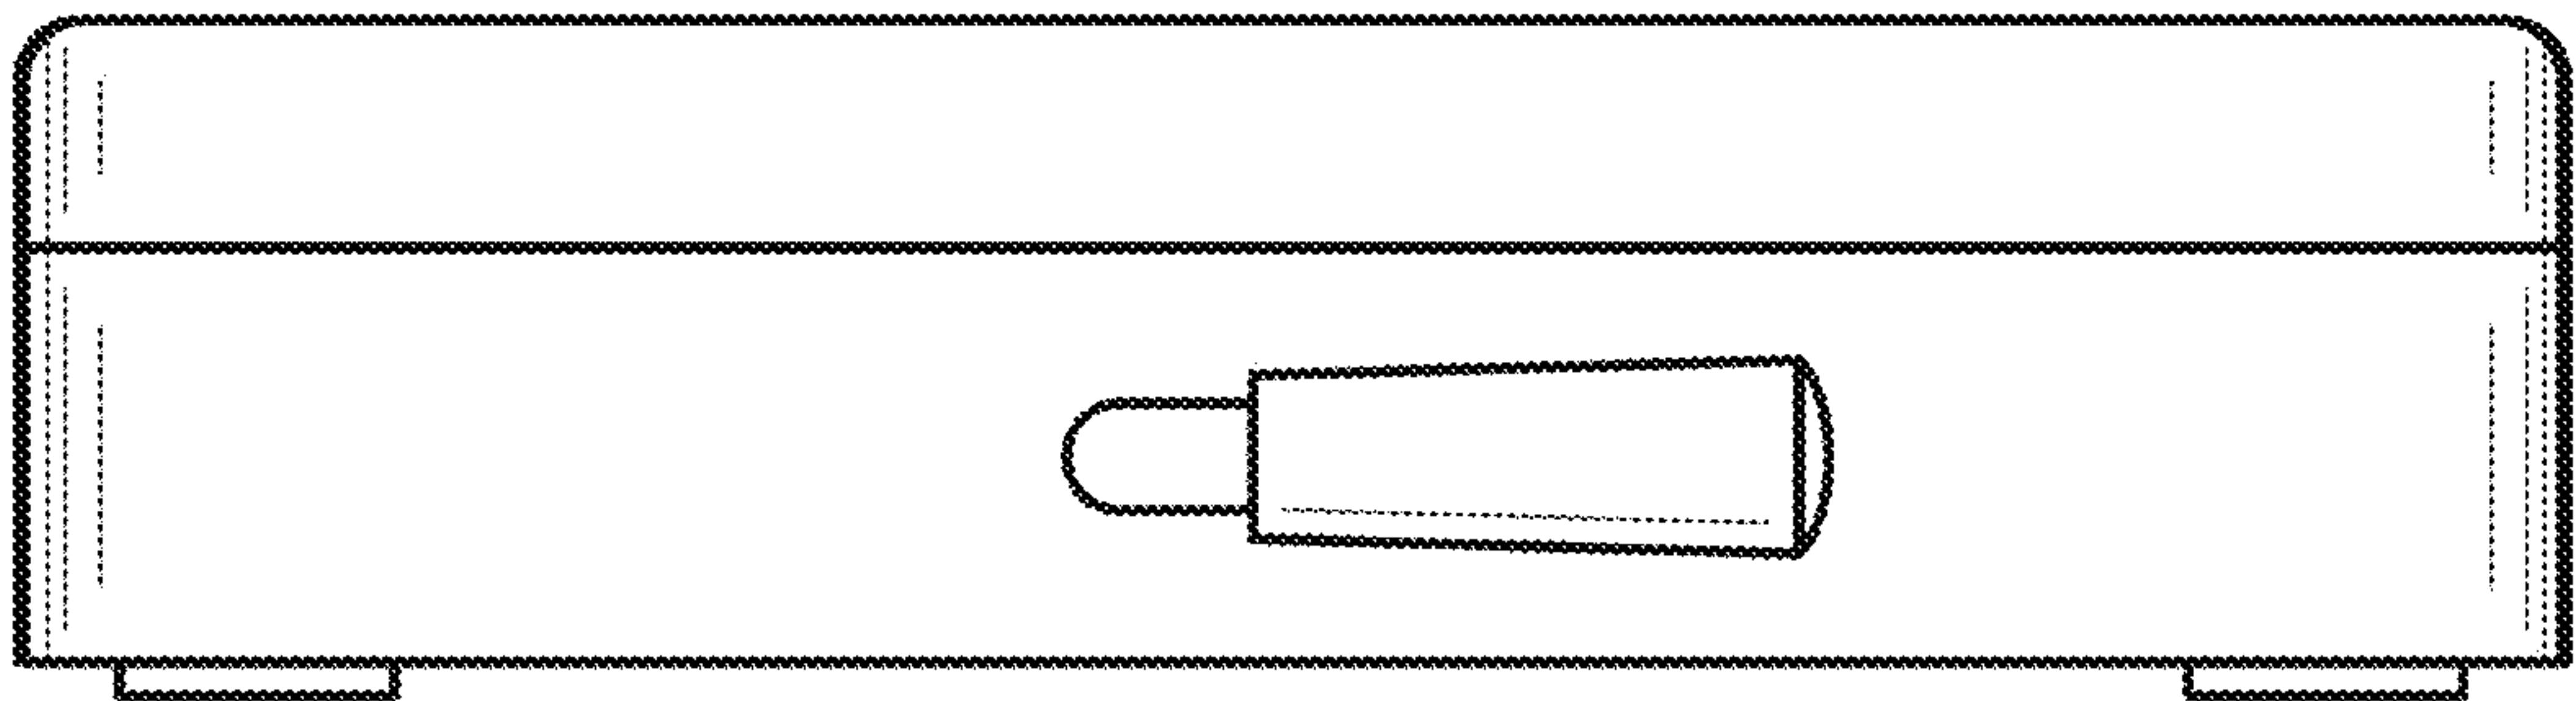


FIG. 5

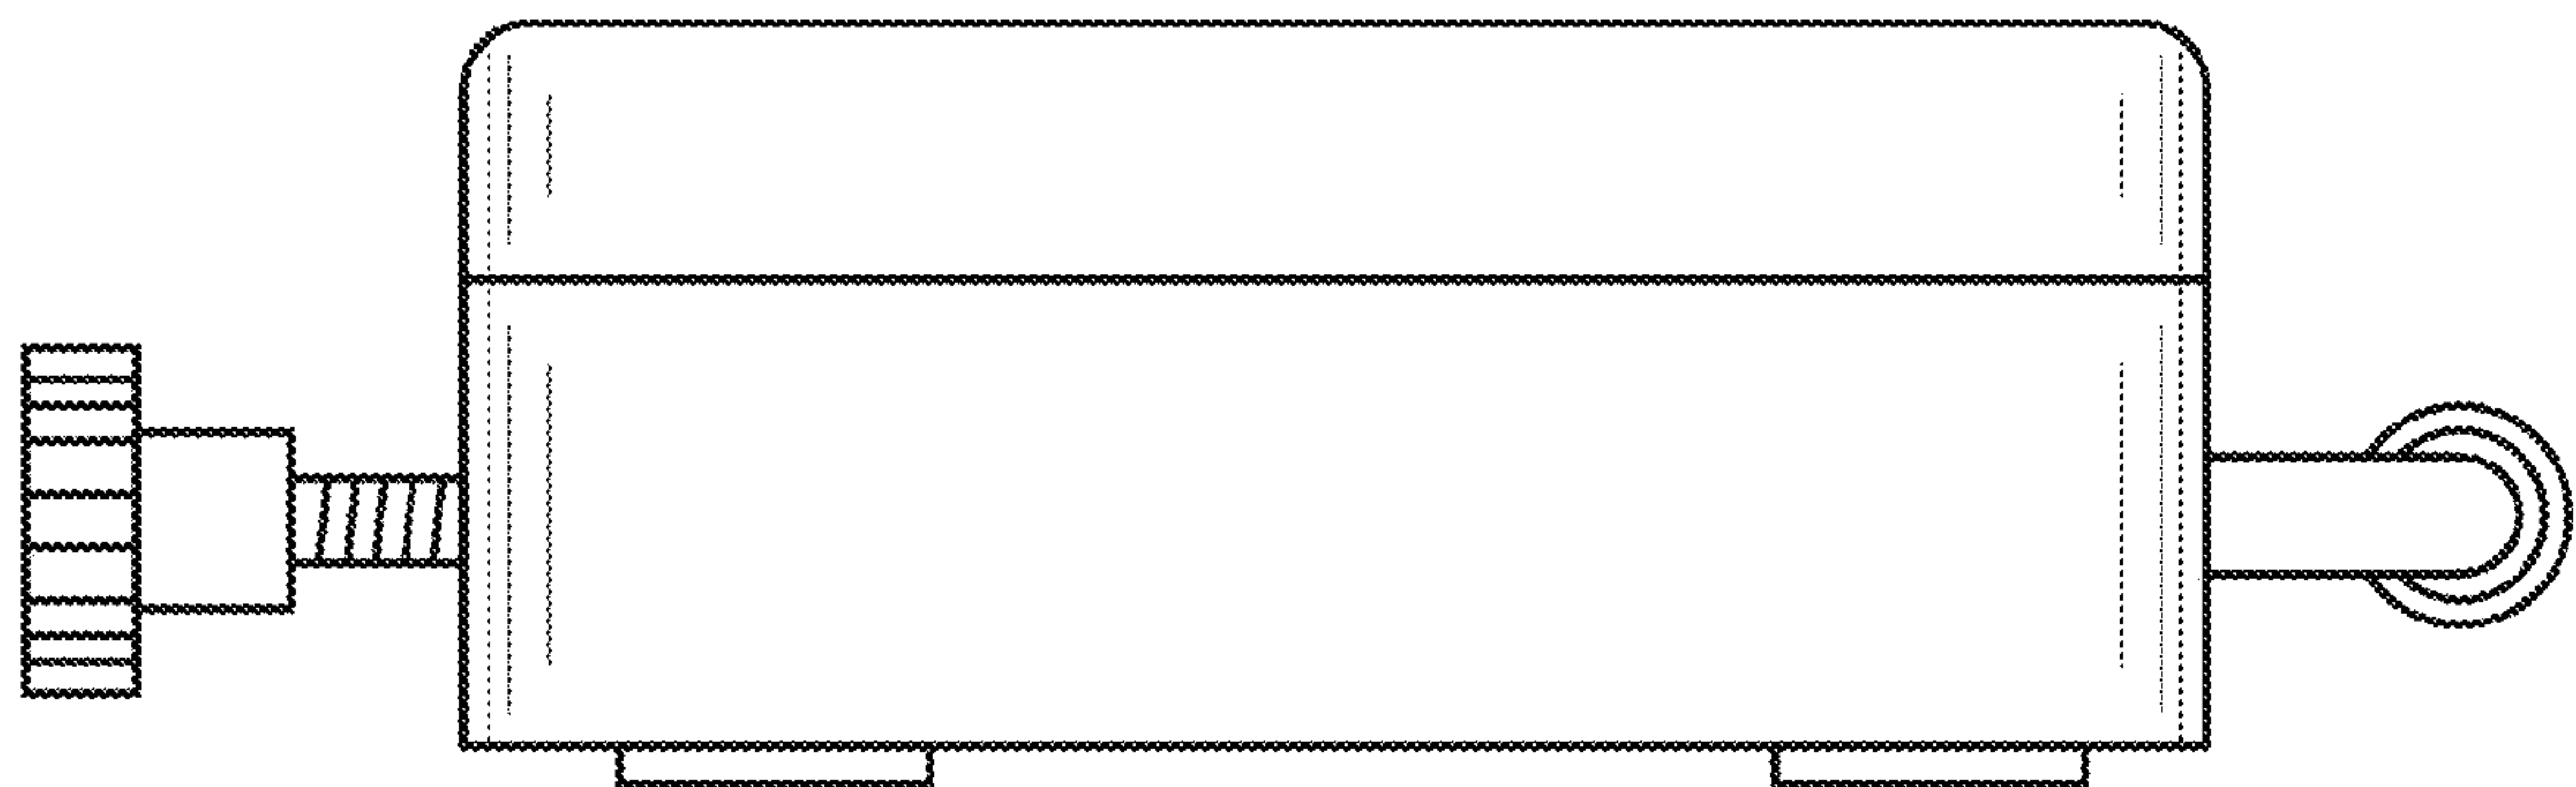


FIG. 6

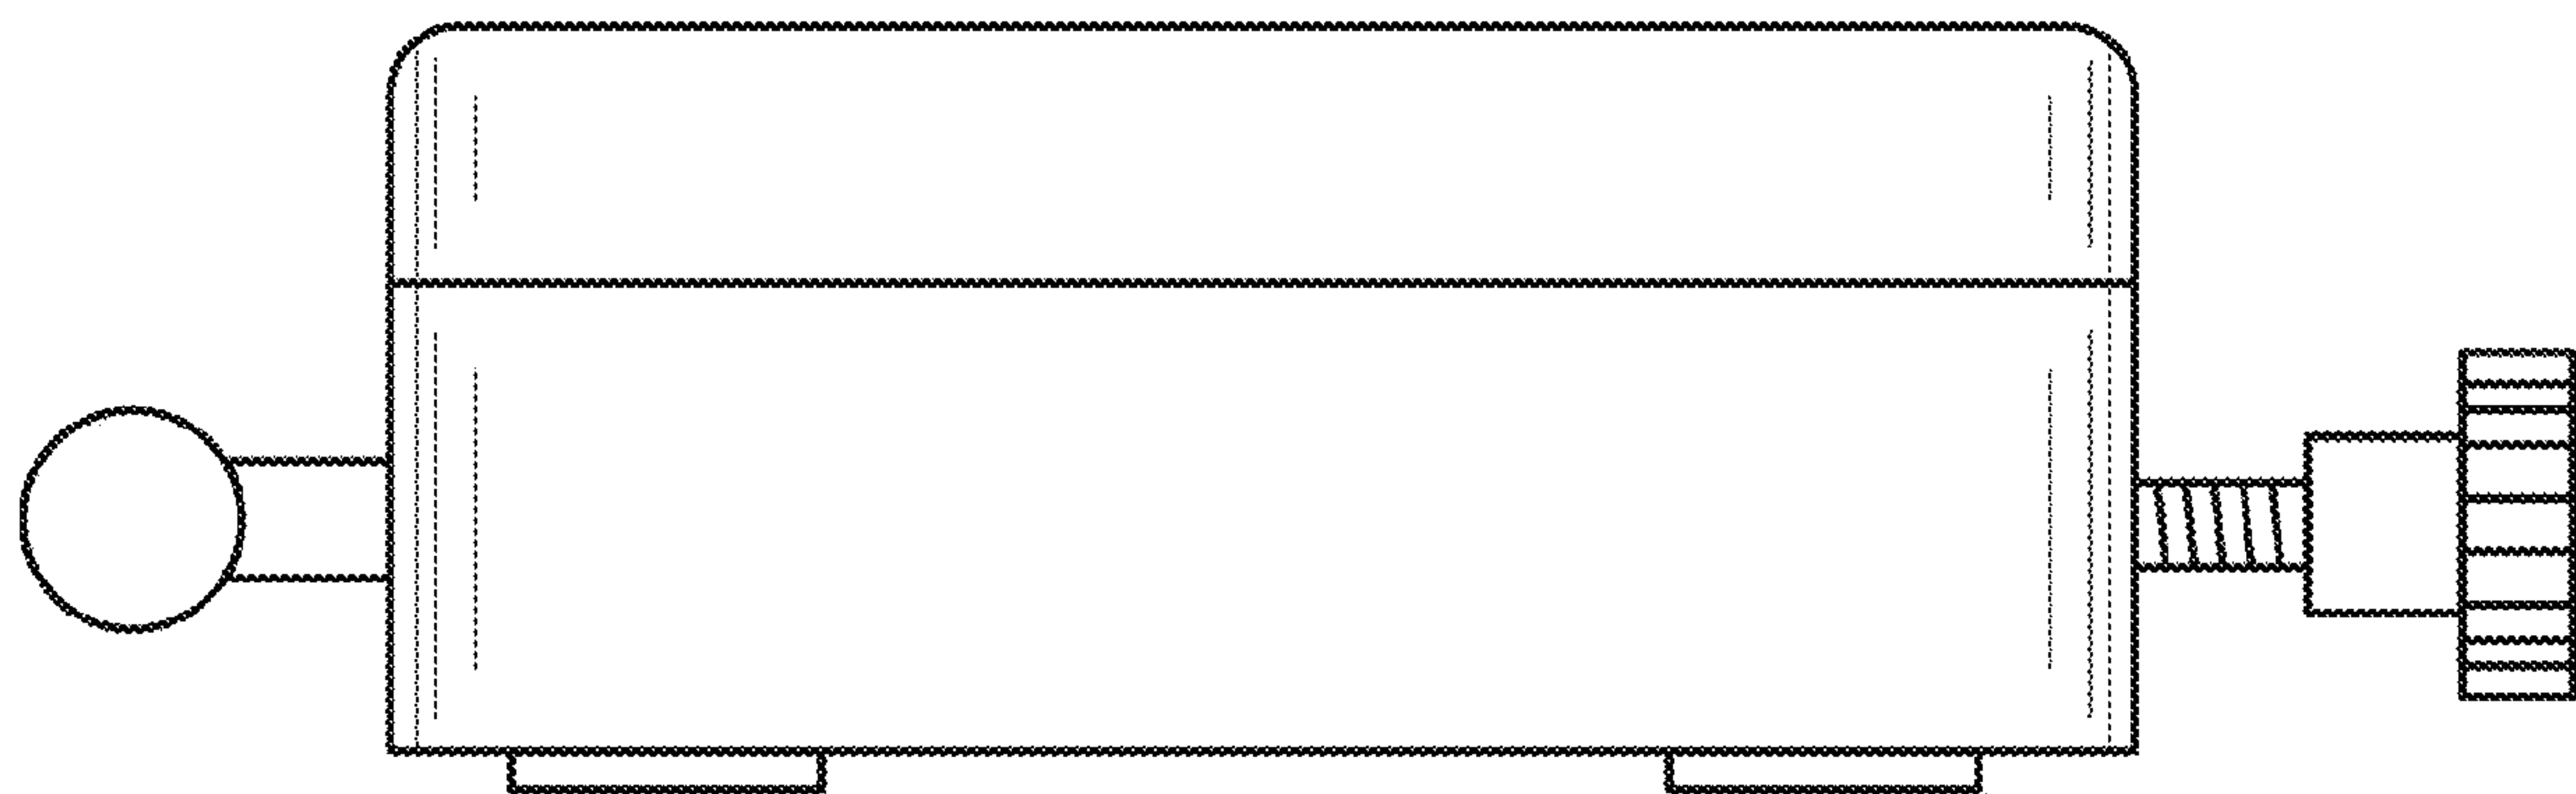


FIG. 7