

(12) **United States Design Patent**
Wheeler et al.

(10) **Patent No.:** **US D1,025,365 S**
(45) **Date of Patent:** **** Apr. 30, 2024**

(54) **RESUSCITATION SYSTEM**

(71) Applicant: **Engineered Medical Systems, Inc.**,
Indianapolis, IN (US)

(72) Inventors: **Bradley Allen Wheeler**, Martinsville,
IN (US); **Kevin Michael Pac**, Fishers,
IN (US)

(73) Assignee: **Engineered Medical Systems, Inc.**,
Indianapolis, IN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/772,071**

(22) Filed: **Feb. 26, 2021**

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/164**

(58) **Field of Classification Search**
USPC D24/163, 164, 165, 170, 185, 186, 110,
D24/129, 110.5, 110.6, 201, 202, 203,
D24/231, 234
CPC A61D 7/00; A61B 5/0013; A61B 5/0077;
A61G 10/026; A61G 11/00
See application file for complete search history.

2009/0071482 A1 * 3/2009 Huddlestone A61M 16/0078
128/205.13

2015/0096559 A1 4/2015 Duval-Arnould et al.

2015/0352303 A1 12/2015 Godwin

2016/0367781 A1 12/2016 McCollum et al.

2017/0157348 A1 6/2017 Gillespoe et al.

2018/0369526 A1 12/2018 McGowan et al.

2019/0328987 A1 10/2019 Takatori et al.

2020/0222648 A1 7/2020 Alberici et al.

2022/0273897 A1 9/2022 Weingart et al.

OTHER PUBLICATIONS

Getting Ready to Use a Manual Resuscitator on a Patient for Manual Ventilation. Apr. 28, 2017. Site visited Sep. 15, 2023. [https://www.youtube.com/watch?v=AK7O-fc3AE8] (Year: 2017).*

Wheeler, B. A. et al., Design U.S. Appl. No. 29/772,065, filed Feb. 26, 2021.

* cited by examiner

Primary Examiner — Wendy L Arminio
Assistant Examiner — Maheen Khurshid
(74) *Attorney, Agent, or Firm* — Woodard, Emhardt,
Henry, Reeves & Wagner, LLP

(57) **CLAIM**

The ornamental design for a resuscitation system, as shown and described.

DESCRIPTION

FIG. 1 is a front, right, perspective view showing our new design;
FIG. 2 is a front side view thereof;
FIG. 3 is a right side view thereof;
FIG. 4 is a back side view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a top view thereof; and,
FIG. 7 is a bottom view thereof.
The broken lines illustrate portions of the resuscitation system that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

D335,552 S * 5/1993 Kohnke D24/110.5

D635,675 S 4/2011 Thompson et al.

9,132,253 B2 9/2015 Lynn et al.

D760,376 S 6/2016 Korneliussen et al.

9,517,316 B2 * 12/2016 Peace A61M 16/0816

D779,071 S 2/2017 Warner, III

10,016,570 B2 * 7/2018 Navarijo A61M 16/0078


11,129,950 B2 * 9/2021 Mielcarz A61M 16/0003

D995,794 S * 8/2023 Rose D24/186

D996,601 S * 8/2023 Ratner D24/110

2001/0029950 A1 10/2001 Haubeil

2008/0087285 A1 4/2008 Kuo

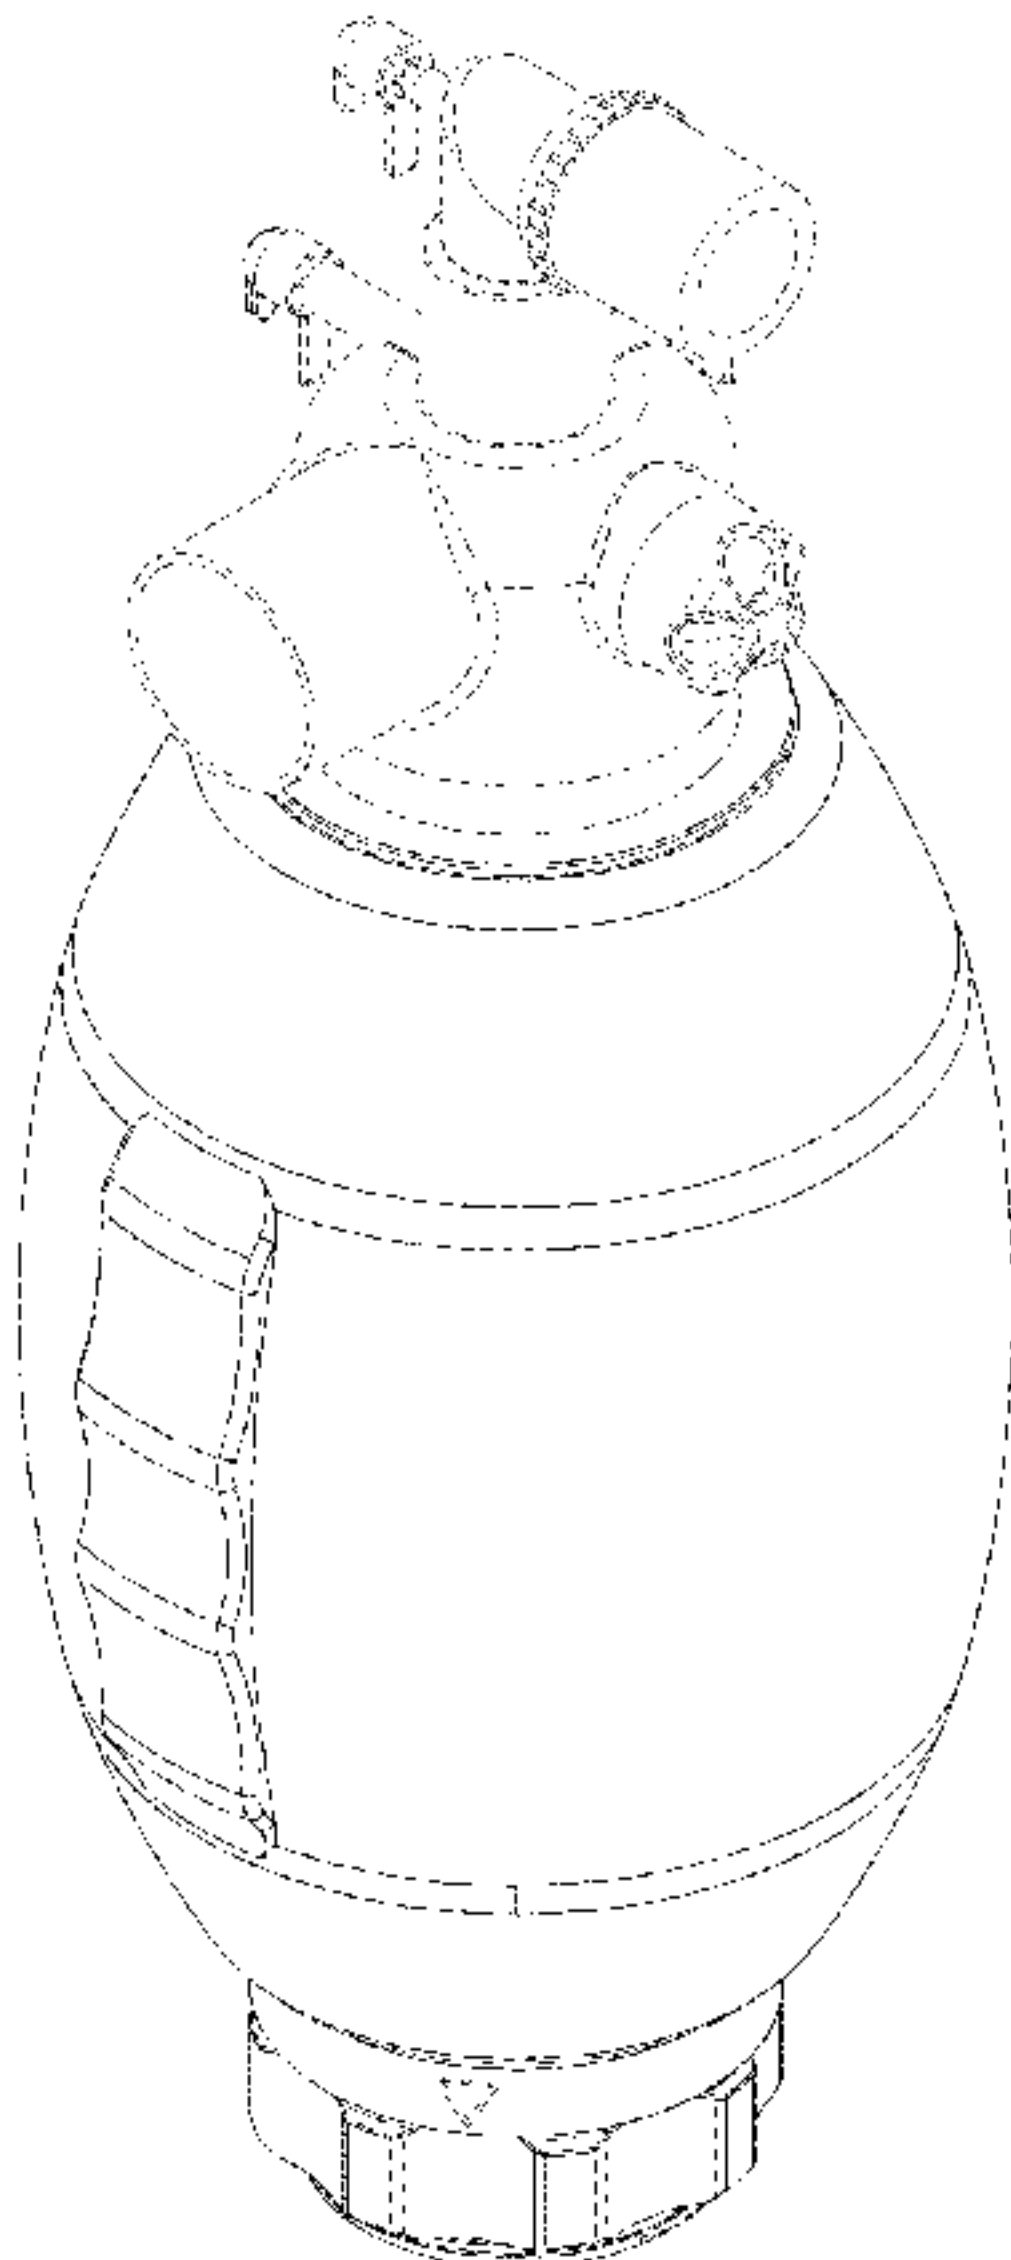

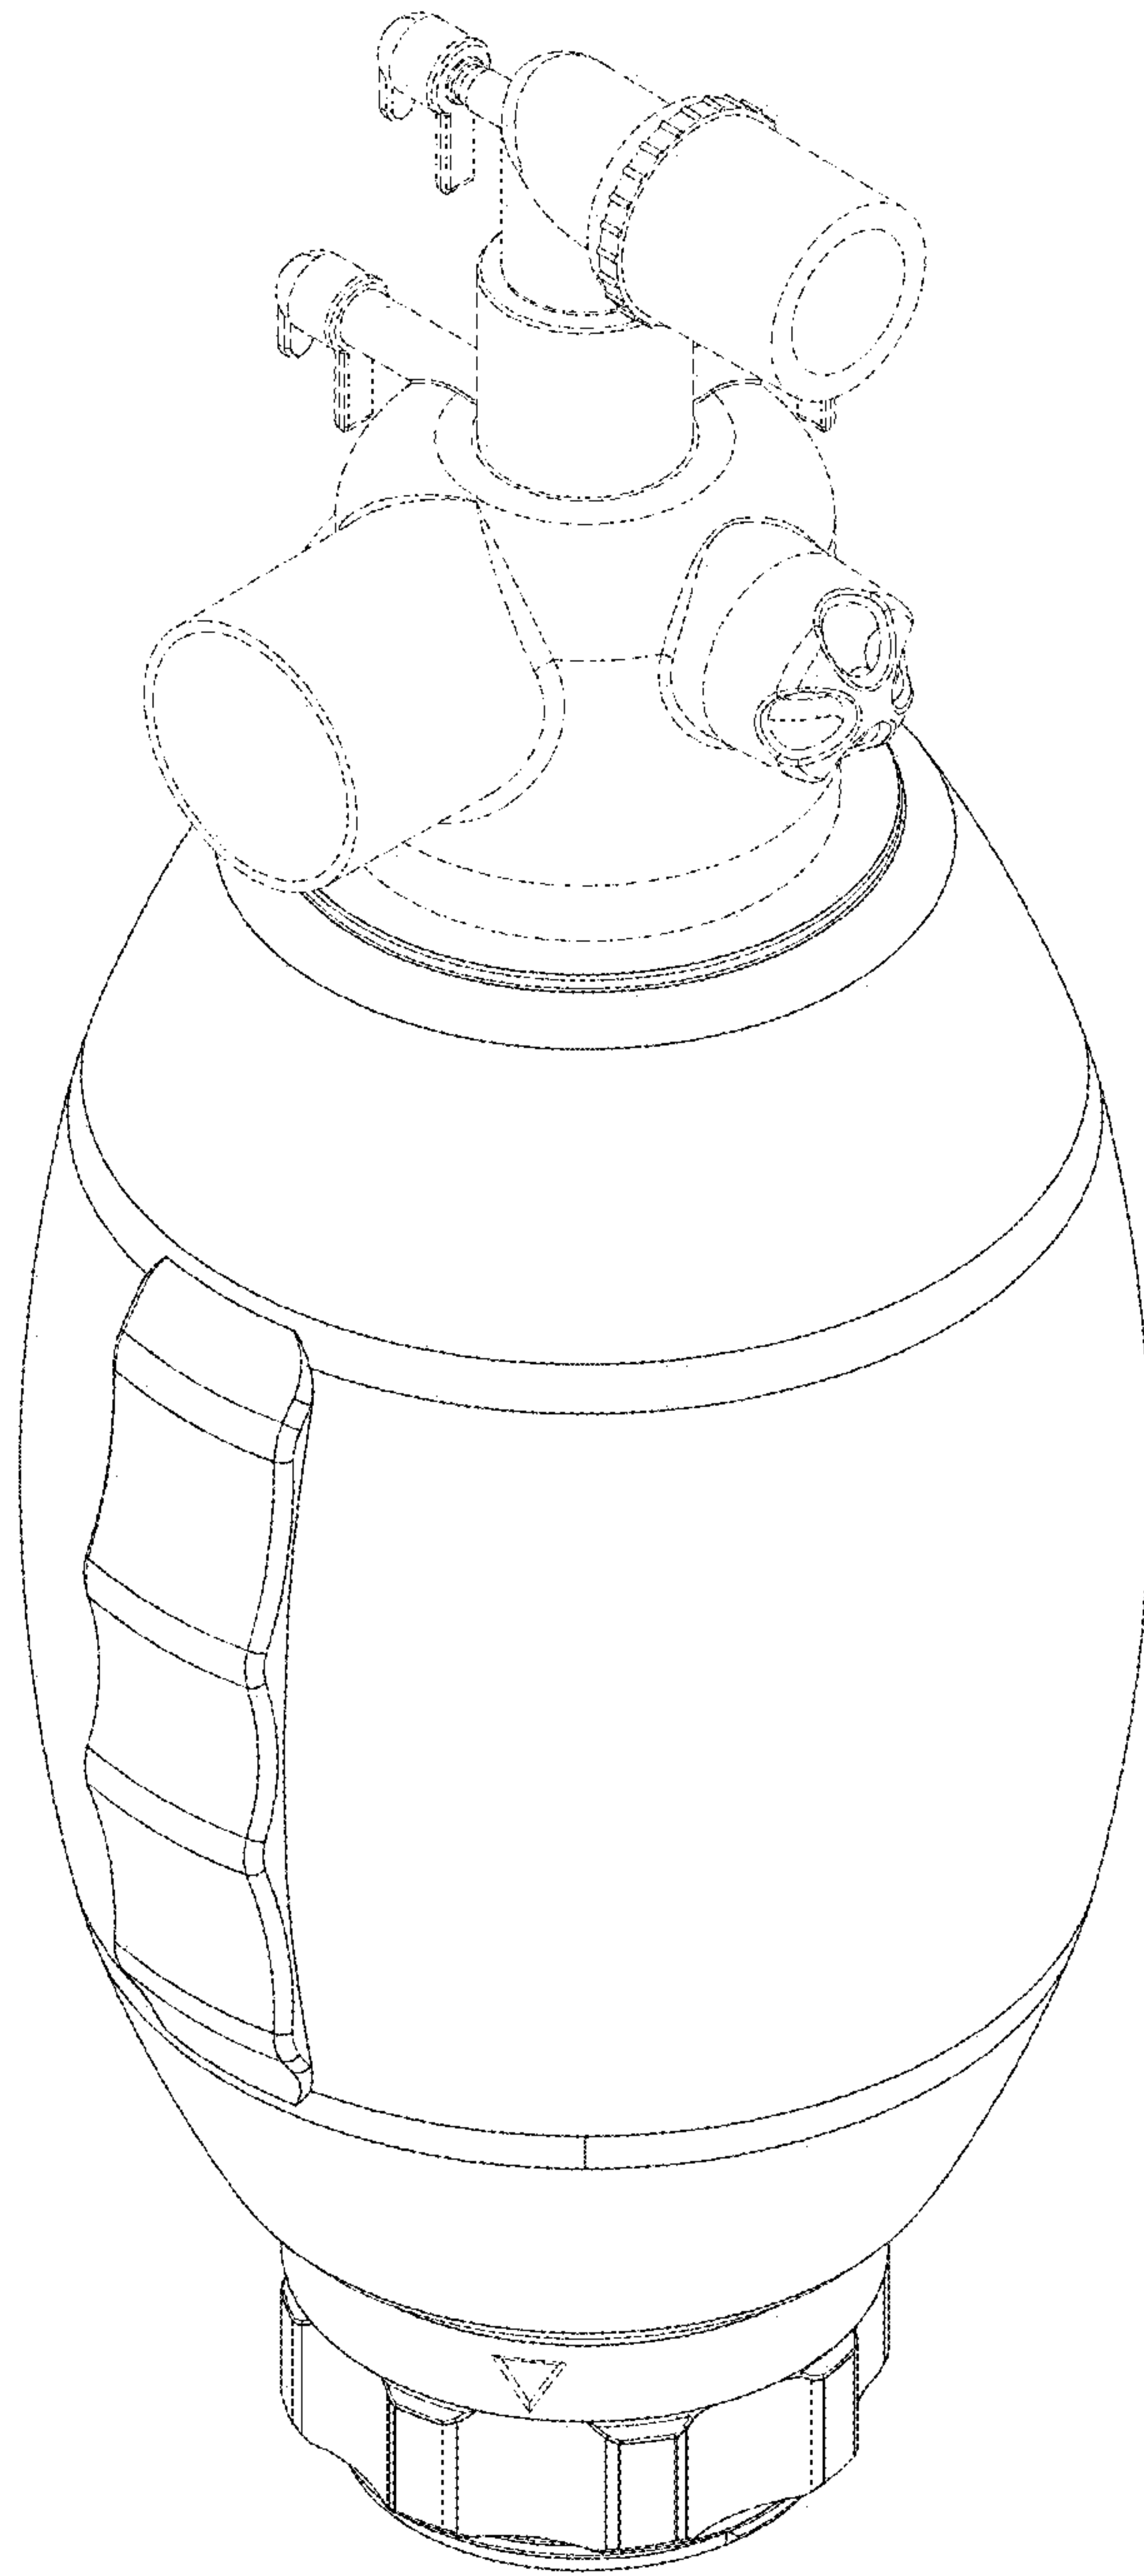


Fig. 1

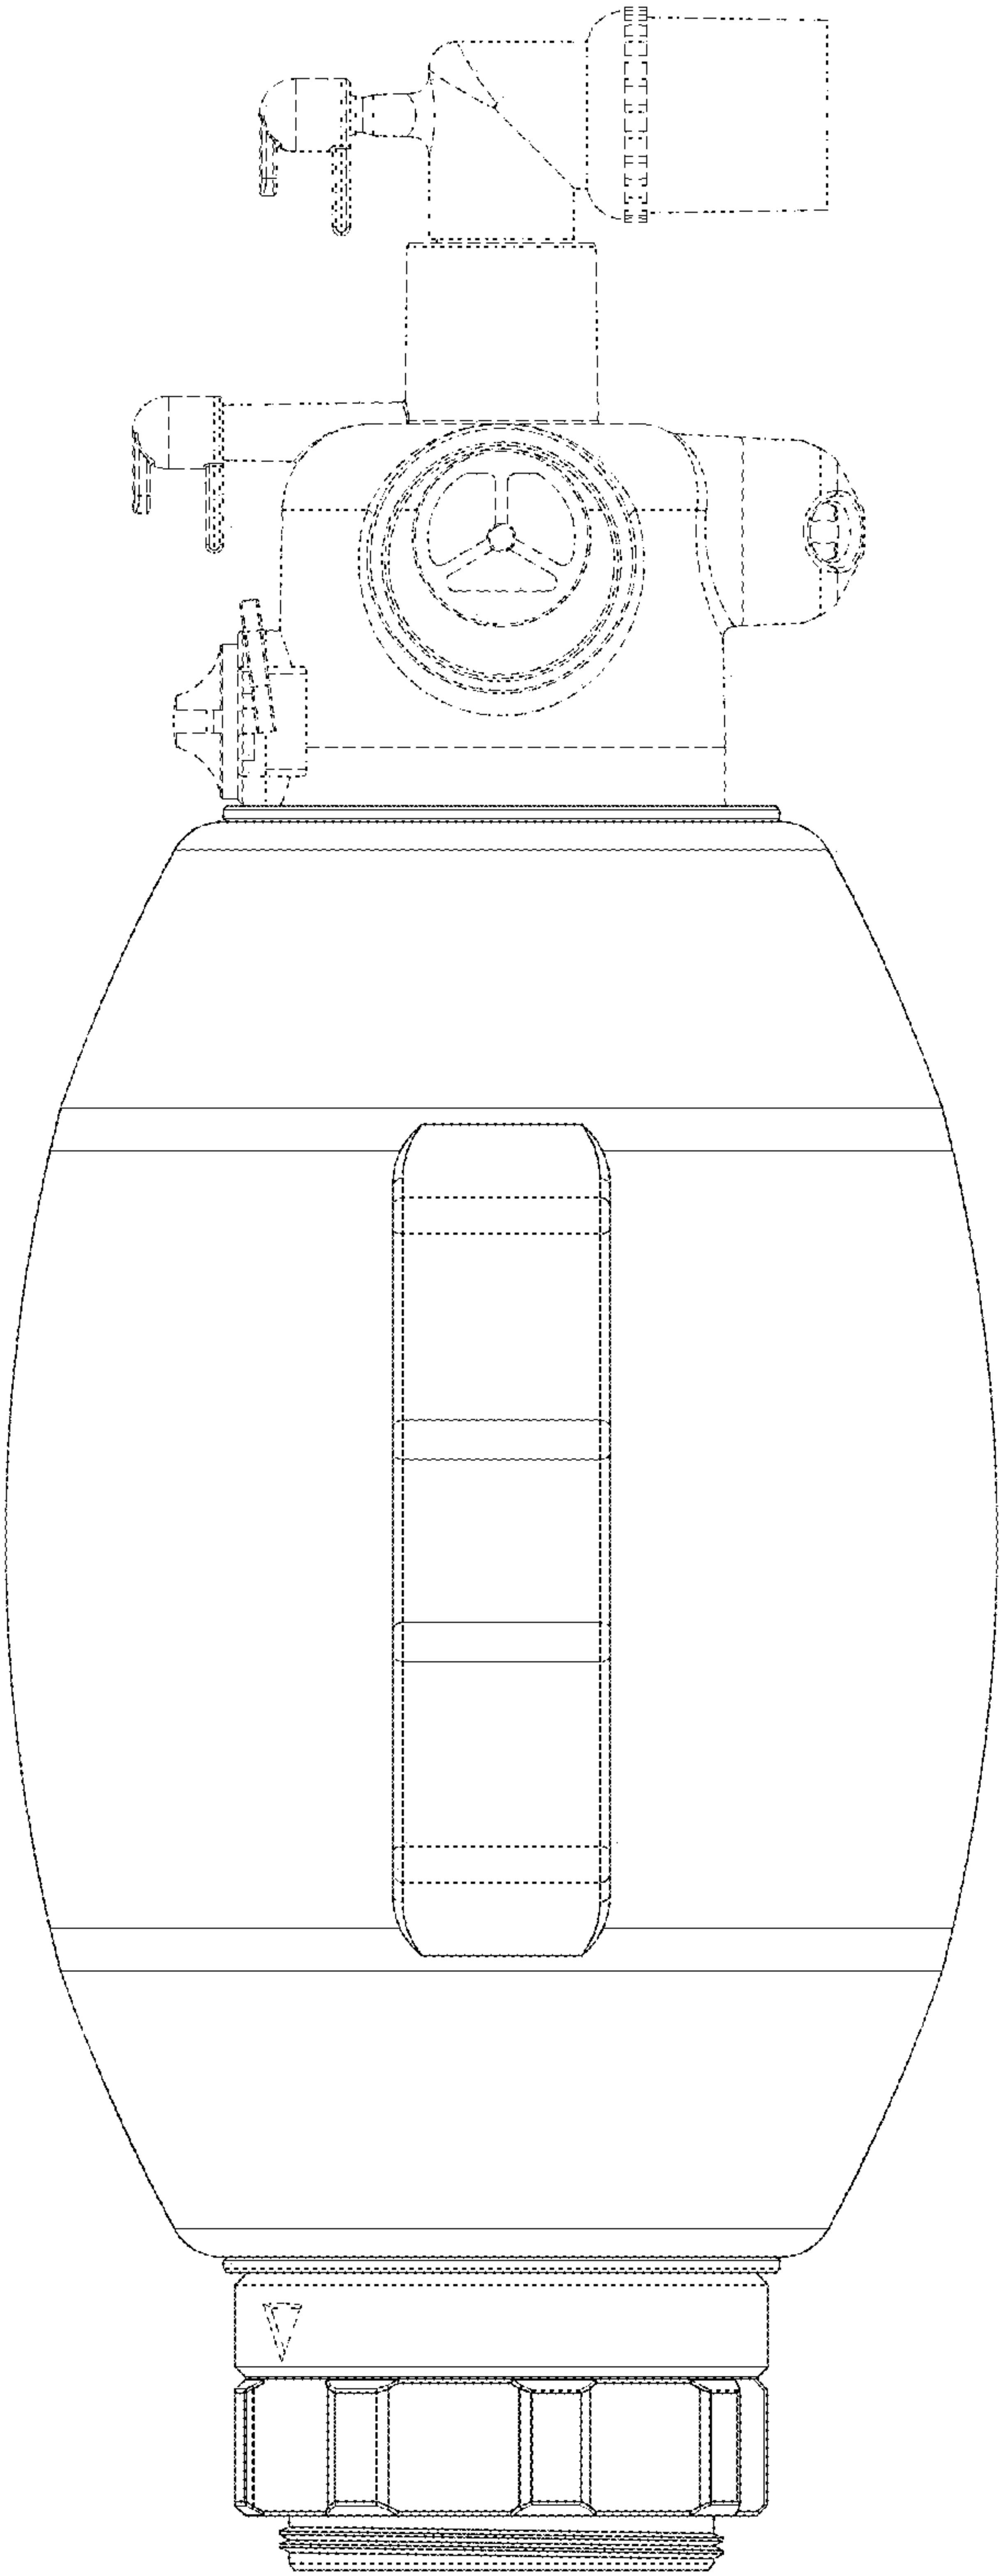


Fig. 2

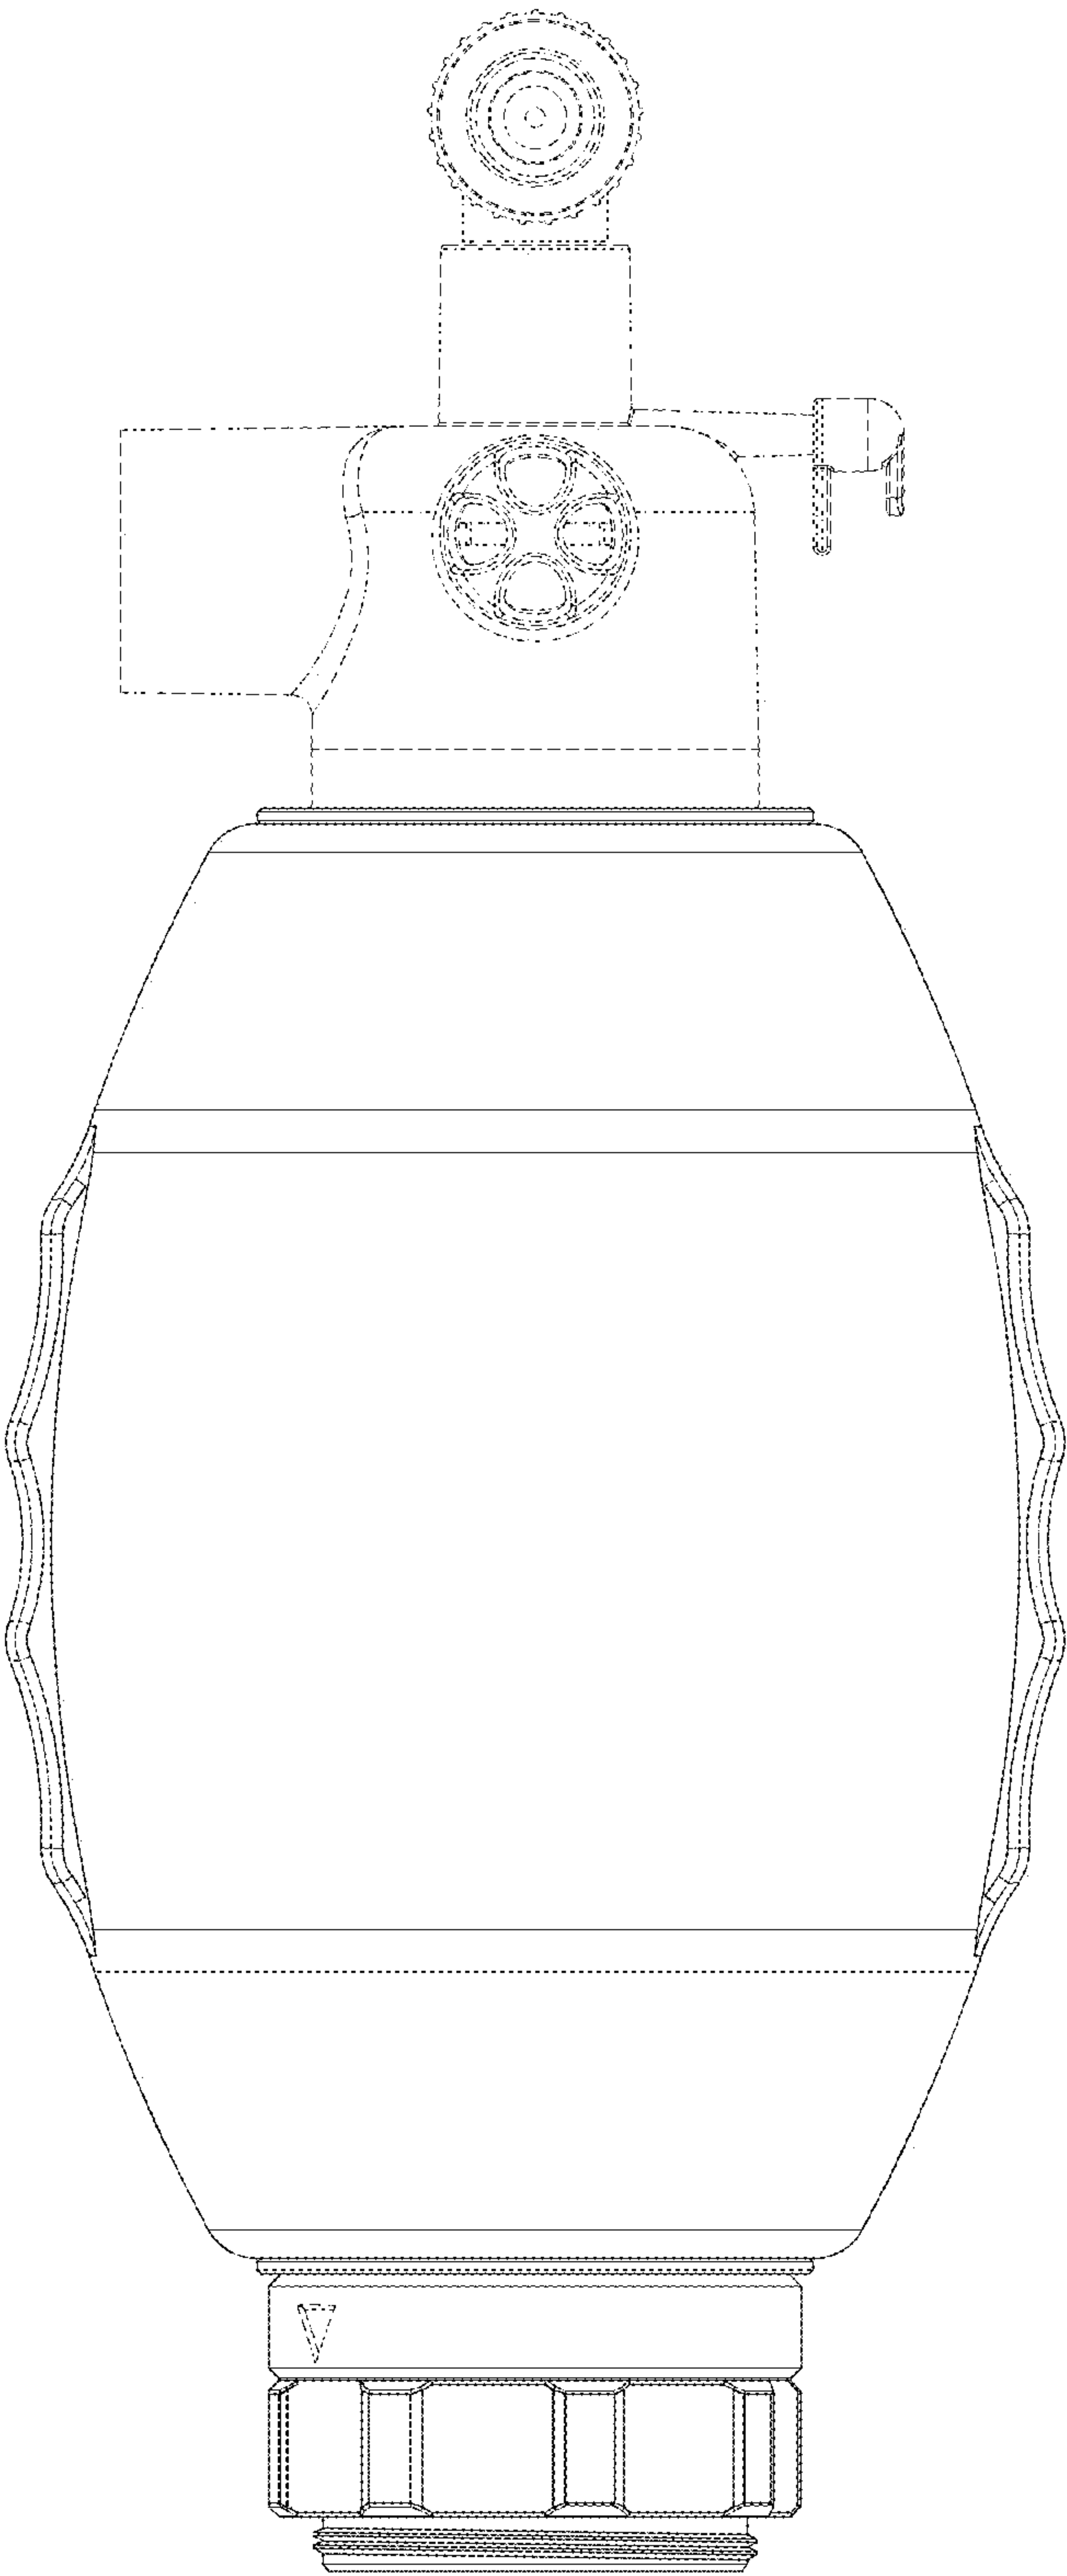


Fig. 3

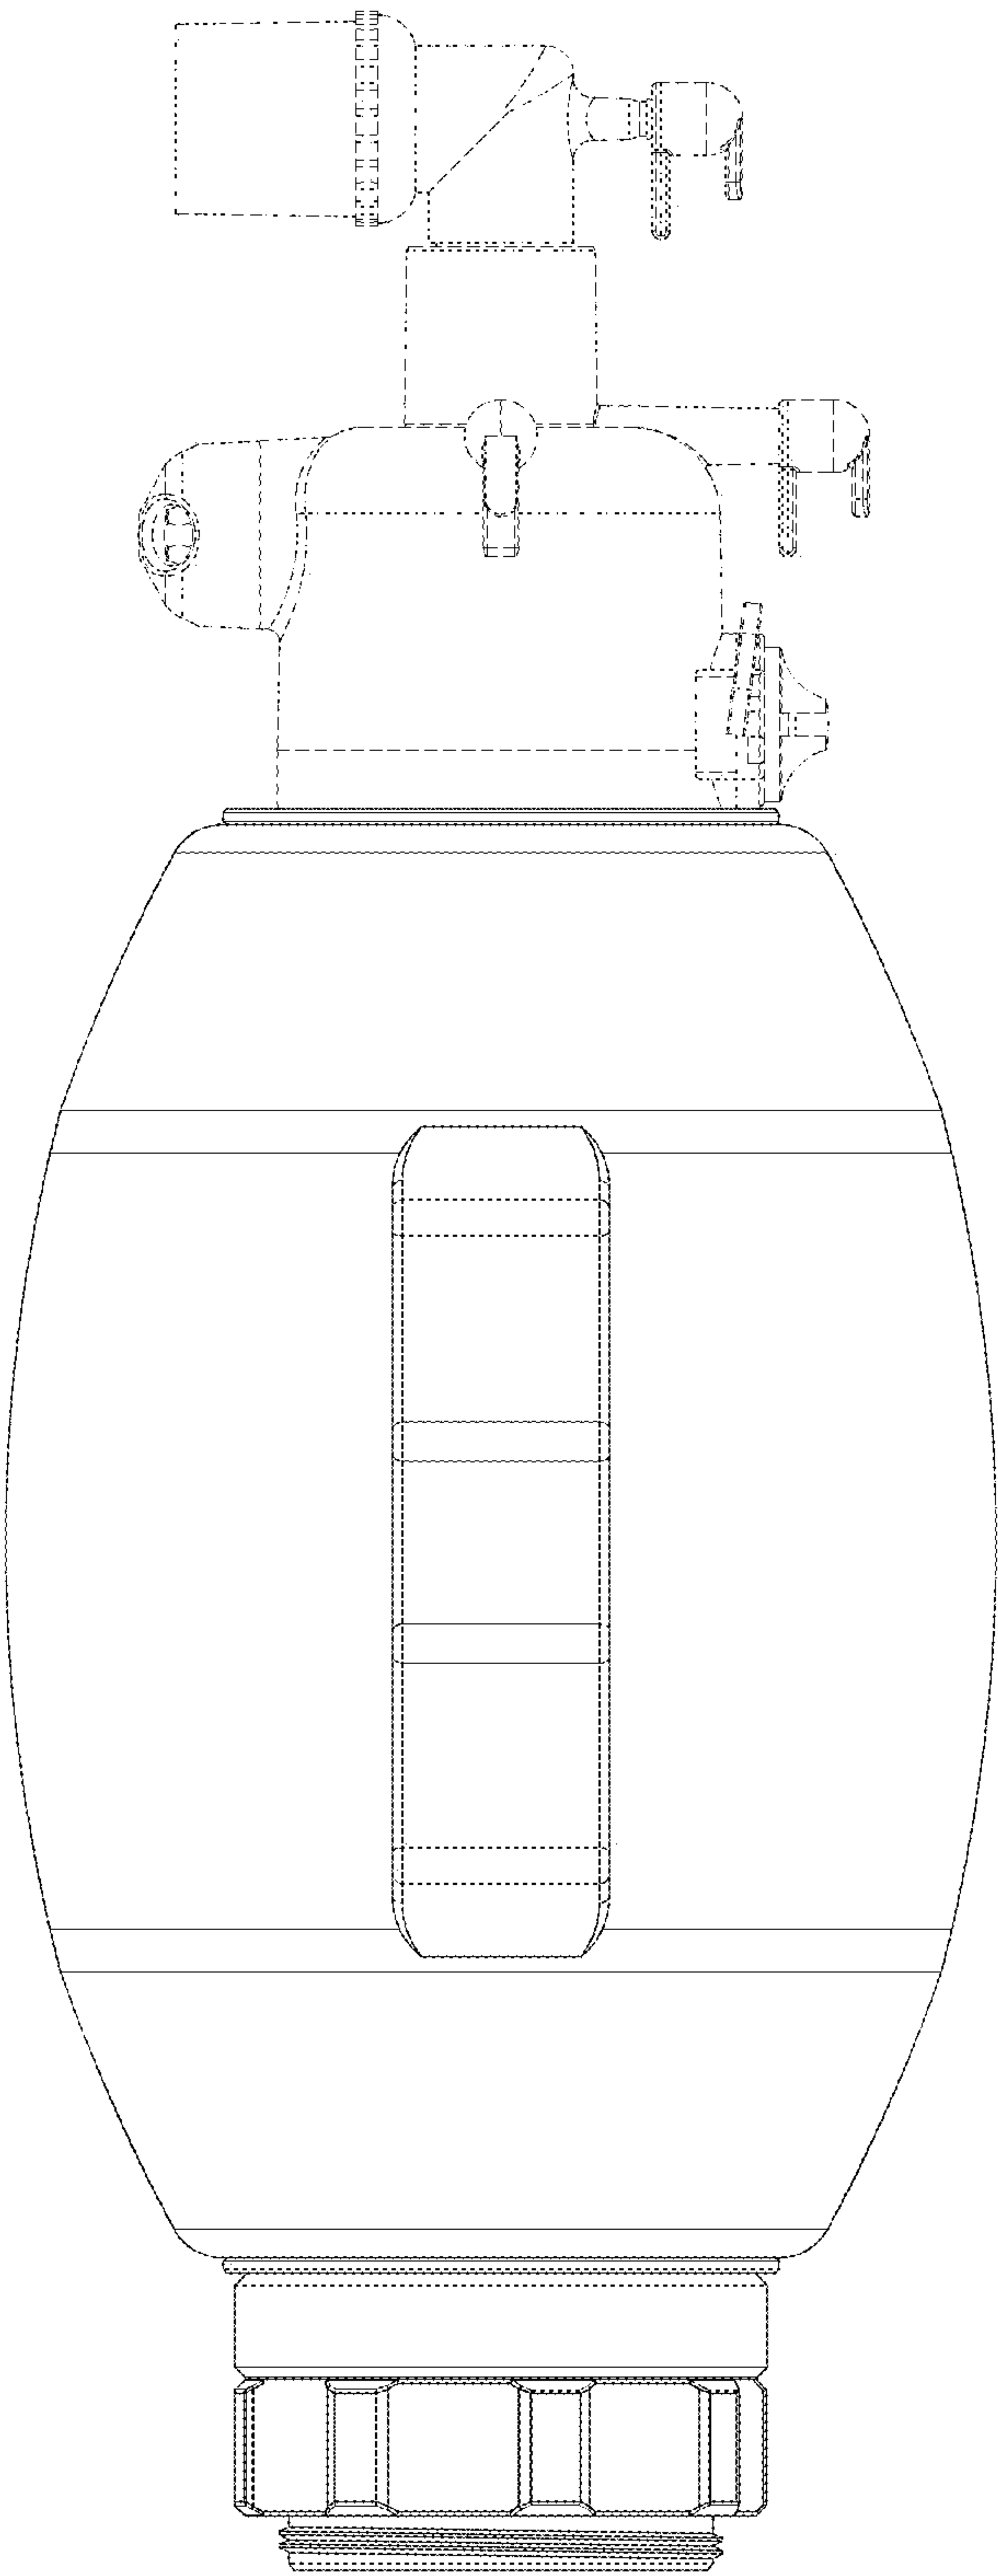


Fig. 4

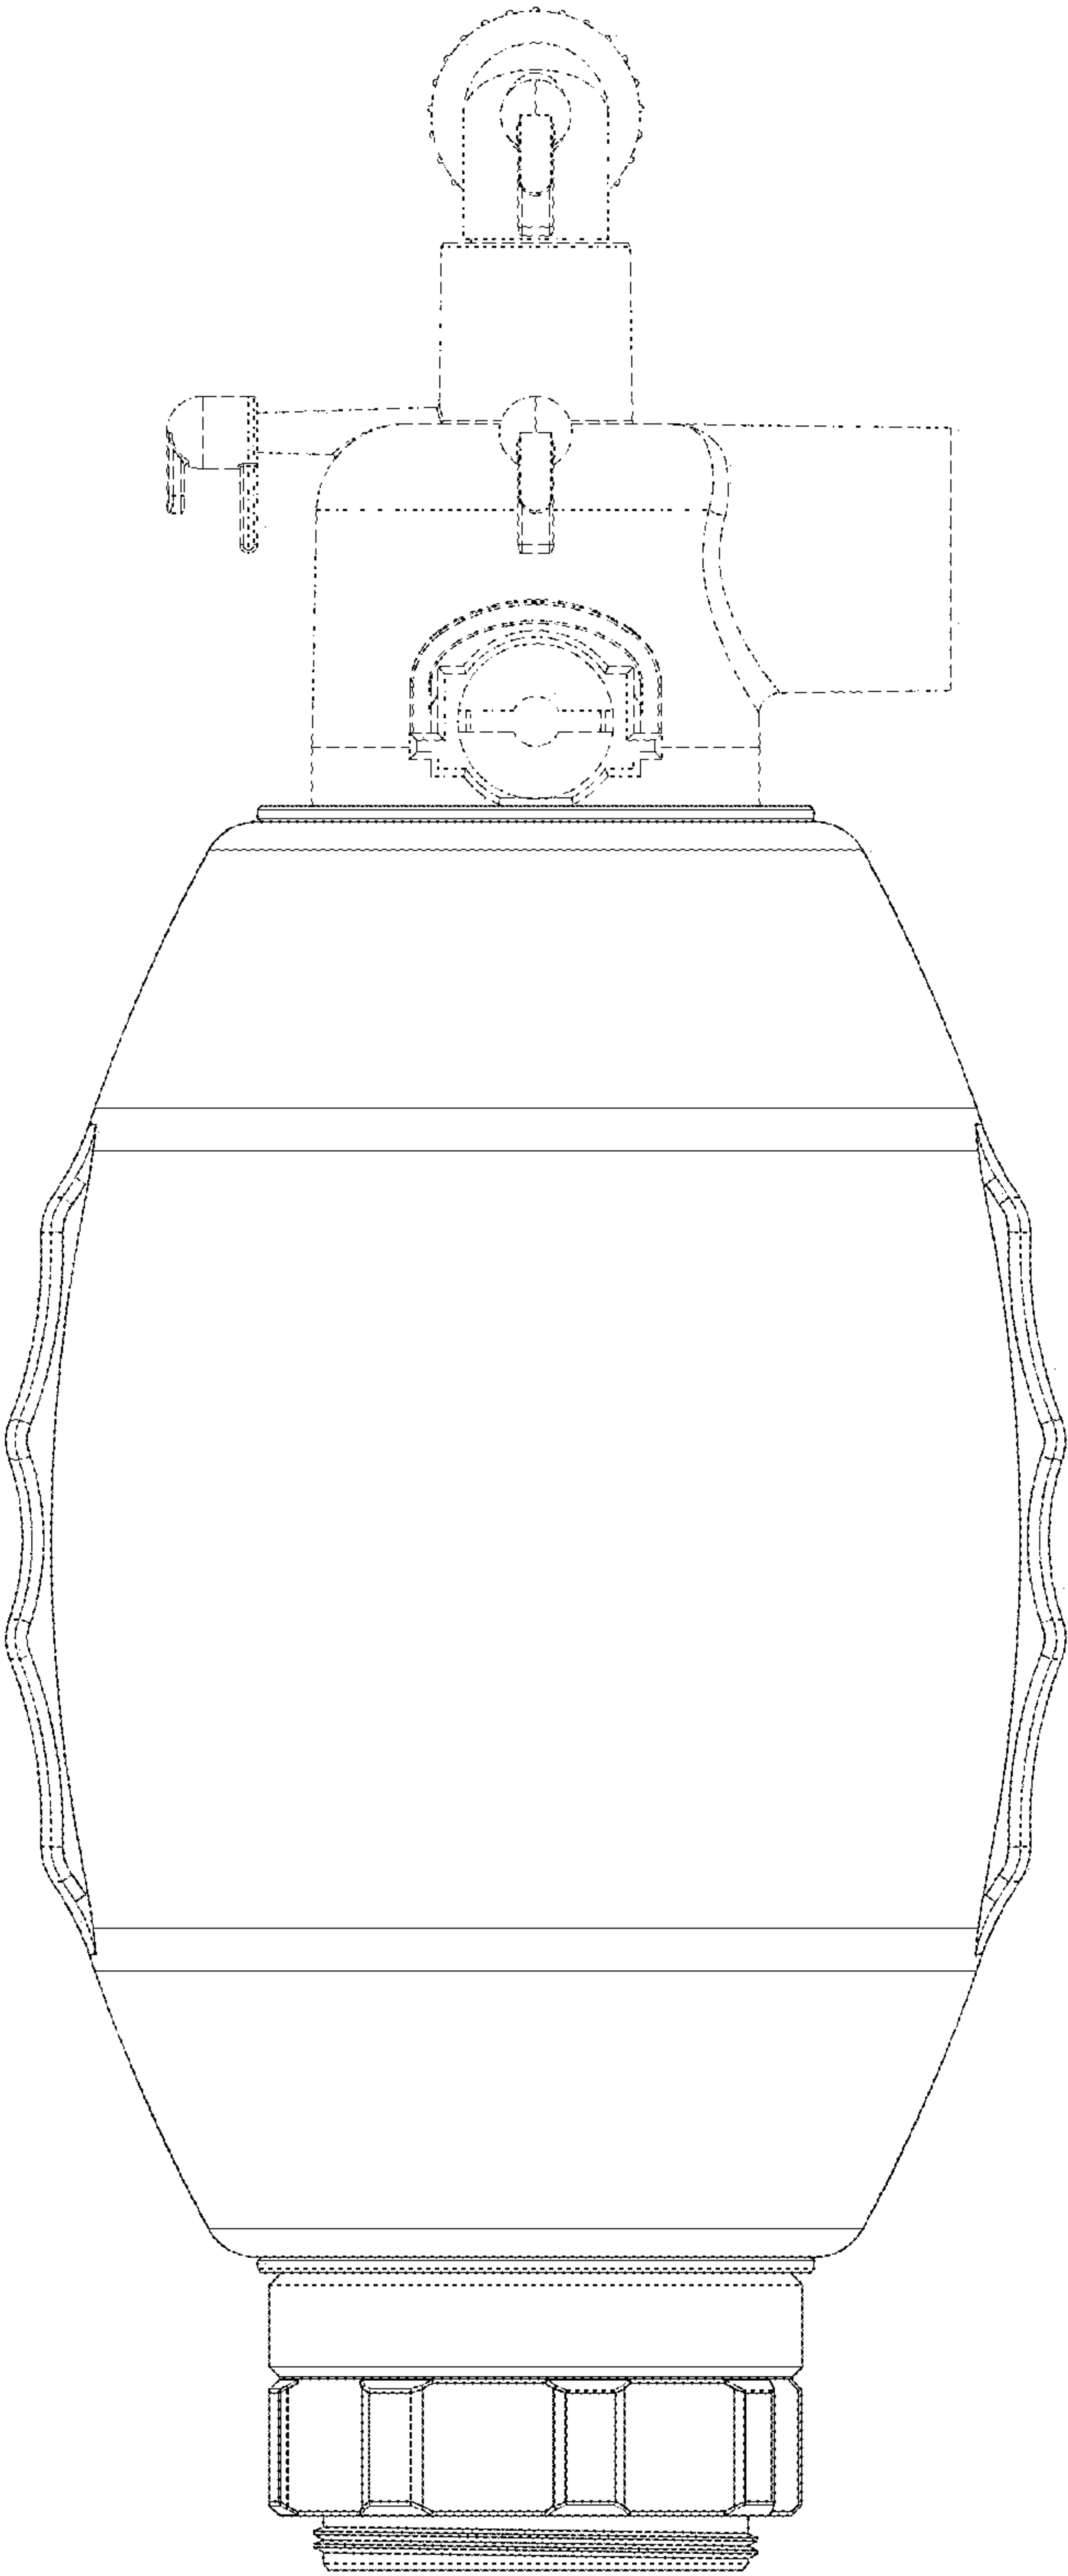


Fig. 5

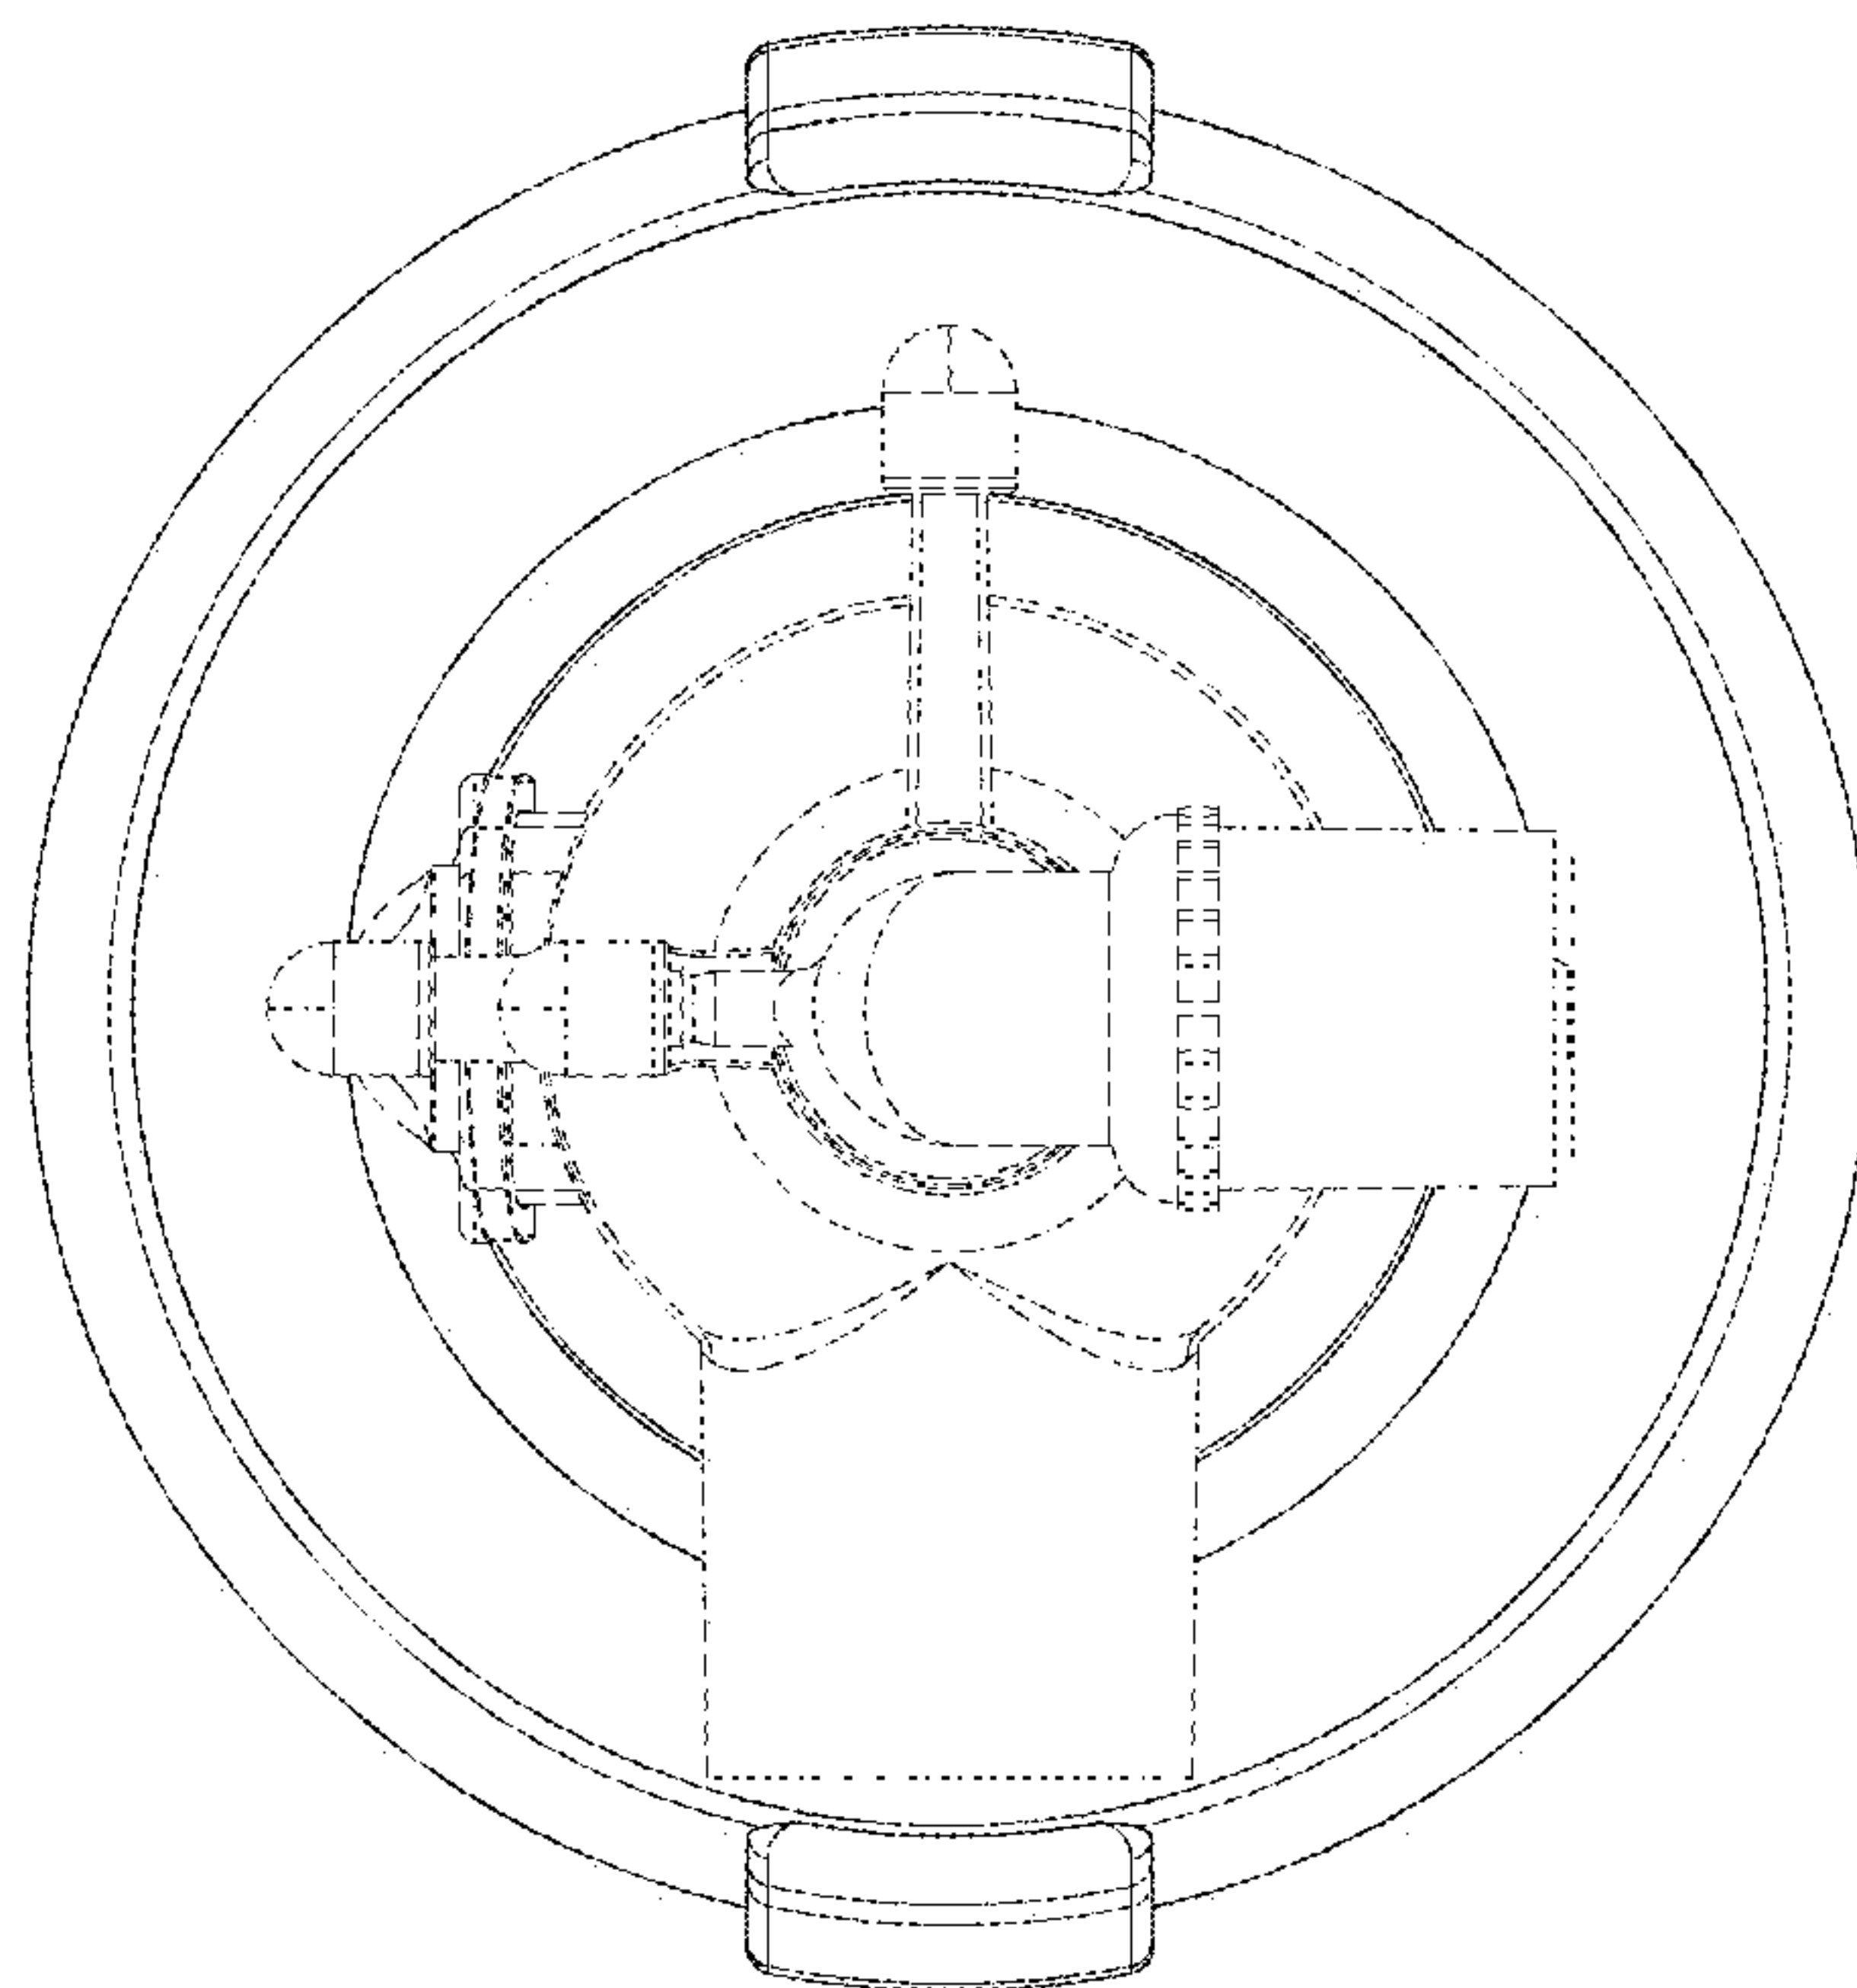


Fig. 6

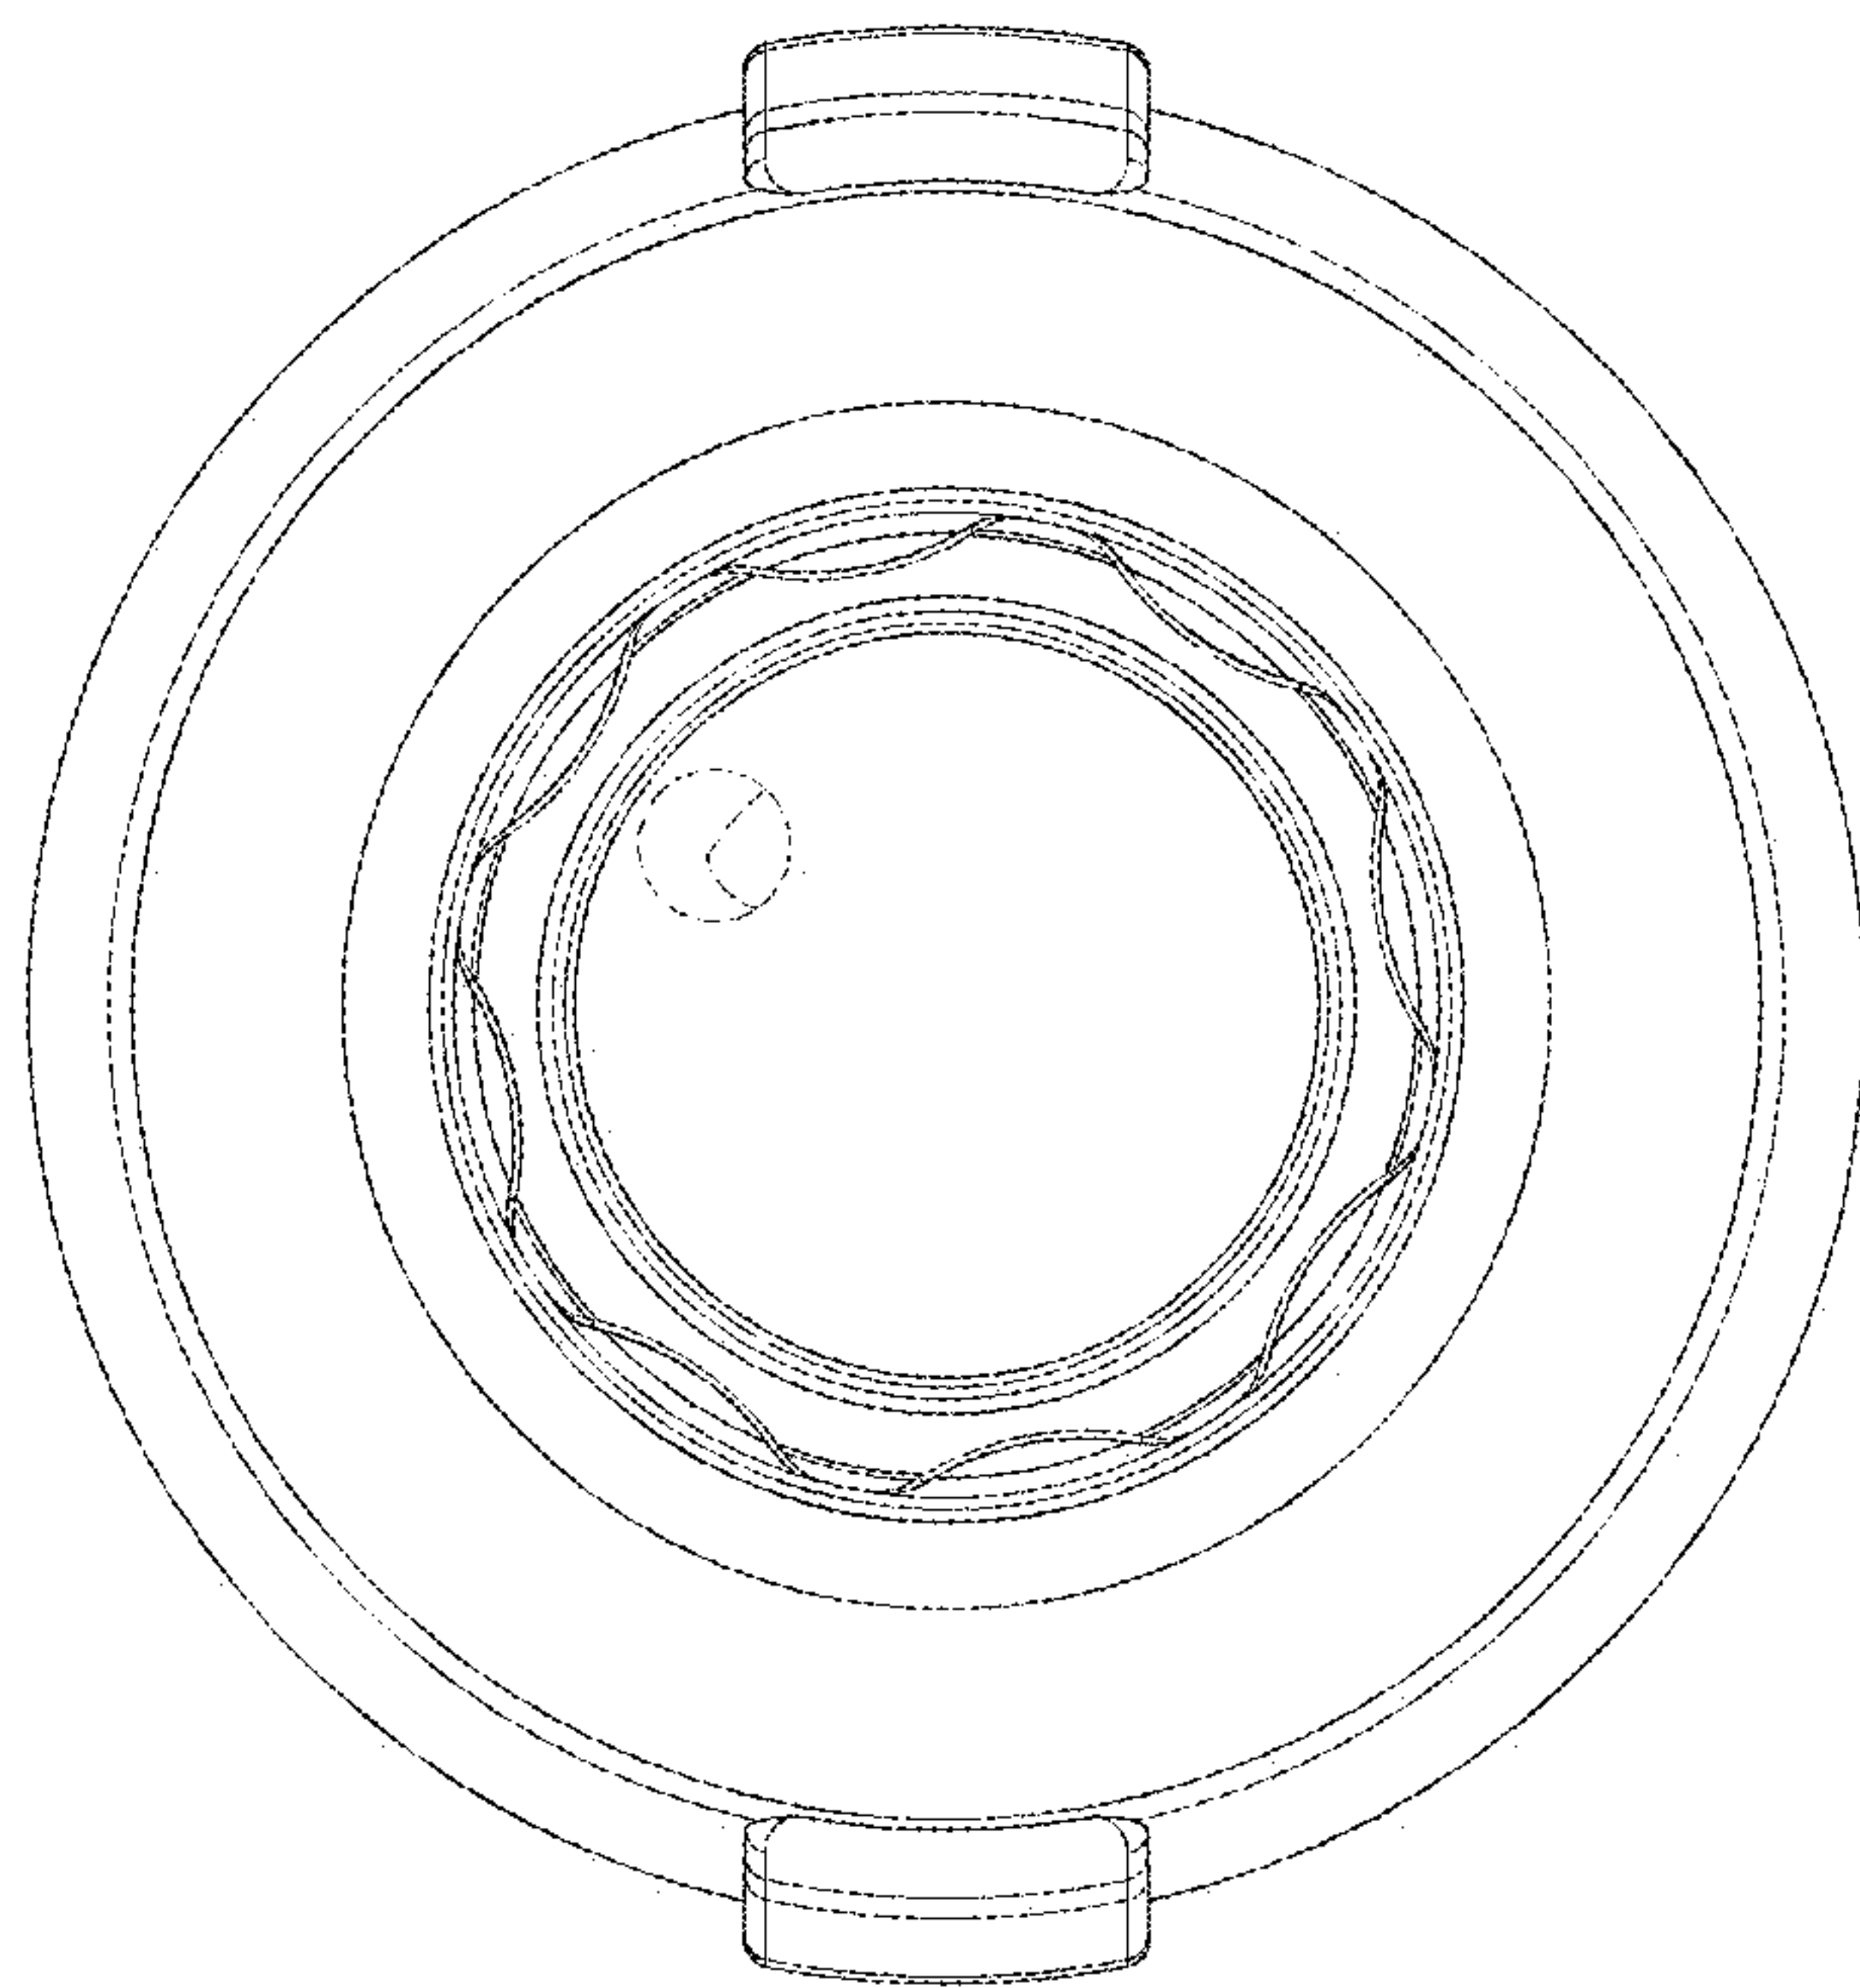


Fig. 7