



US0D1026244S

(12)

United States Design Patent

Chang et al.

(10) Patent No.:

US D1,026,244 S

(45) Date of Patent:

** May 7, 2024

(54) DIAGNOSTIC ASSAY SYSTEM

(71) Applicant: Cepheid, Sunnyvale, CA (US)

(72) Inventors: Ronald Chang, Redwood City, CA (US); Gregory Mote, Sunnyvale, CA (US); Steven M. Montgomery, Sunnyvale, CA (US)

(73) Assignee: Cepheid, Sunnyvale, CA (US)

(**) Term: 15 Years

(21) Appl. No.: 29/865,799

(22) Filed: Aug. 12, 2022

(51) LOC (14) Cl. 24-01

(52) U.S. Cl. D24/216

(58) Field of Classification Search

USPC D24/107, 169, 185, 186, 209, 210, 216, 224/217, 218, 219, 231–234, 223; D10/81; D14/420

CPC G01N 35/00306; G01N 35/00326; G01N 35/00336; G01N 35/025; G01N 35/1085; G01N 2021/6432; G01N 21/6458; G01N 21/6484; G01N 21/6486; G01N 21/76; G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 2030/027

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D297,564 S * 9/1988 Yamamoto D24/232

D322,337 S * 12/1991 Padgett D32/1

D354,013 S * 1/1995 Ninomiya D24/232

D588,276 S * 3/2009 Isozaki D24/232

D616,563 S * 5/2010 Huck D24/217

D670,401 S * 11/2012 Tsuda D24/216

D681,233 S * 4/2013 Thomas D24/232

D681,844 S * 5/2013 Matsuguma D24/232

D681,845	S	*	5/2013	Matsuguma	D24/232
D684,270	S	*	6/2013	Chang	D24/216
D687,561	S	*	8/2013	Iseki	D24/216
D693,714	S	*	11/2013	Noda	D24/232
D693,938	S	*	11/2013	Matoba	D24/232
D705,441	S	*	5/2014	Chang	D24/216
D705,943	S	*	5/2014	Chang	D24/216
D705,944	S	*	5/2014	Chang	D24/216
D717,460	S	*	11/2014	Manian	D24/216
D745,184	S	*	12/2015	Giusti	D24/232
D750,271	S	*	2/2016	Oonuma	D24/216

(Continued)

Primary Examiner — T Chase Nelson

Assistant Examiner — Kelly L Gross

(74) Attorney, Agent, or Firm — Kilpatrick Townsend & Stockton LLP

(57) CLAIM

The ornamental design for a diagnostic assay system, as shown and described.

DESCRIPTION

FIG. 1 shows a front perspective view of a diagnostic assay system showing our new design;

FIG. 2 shows a rear perspective view of the diagnostic assay system;

FIG. 3 shows a top view of the diagnostic assay system;

FIG. 4 shows a rear view of the diagnostic assay system;

FIG. 5 shows a left side view of the diagnostic assay system;


FIG. 6 shows a right side view of the diagnostic assay system;

FIG. 7 shows a front view of the diagnostic assay system; and,

FIG. 8 shows an underside view of the diagnostic assay system.

The broken lines immediately adjacent the shaded areas represent the bounds of the claim, while all other broken lines are directed to environment; the broken lines form no part of the claimed design.

1 Claim, 8 Drawing Sheets

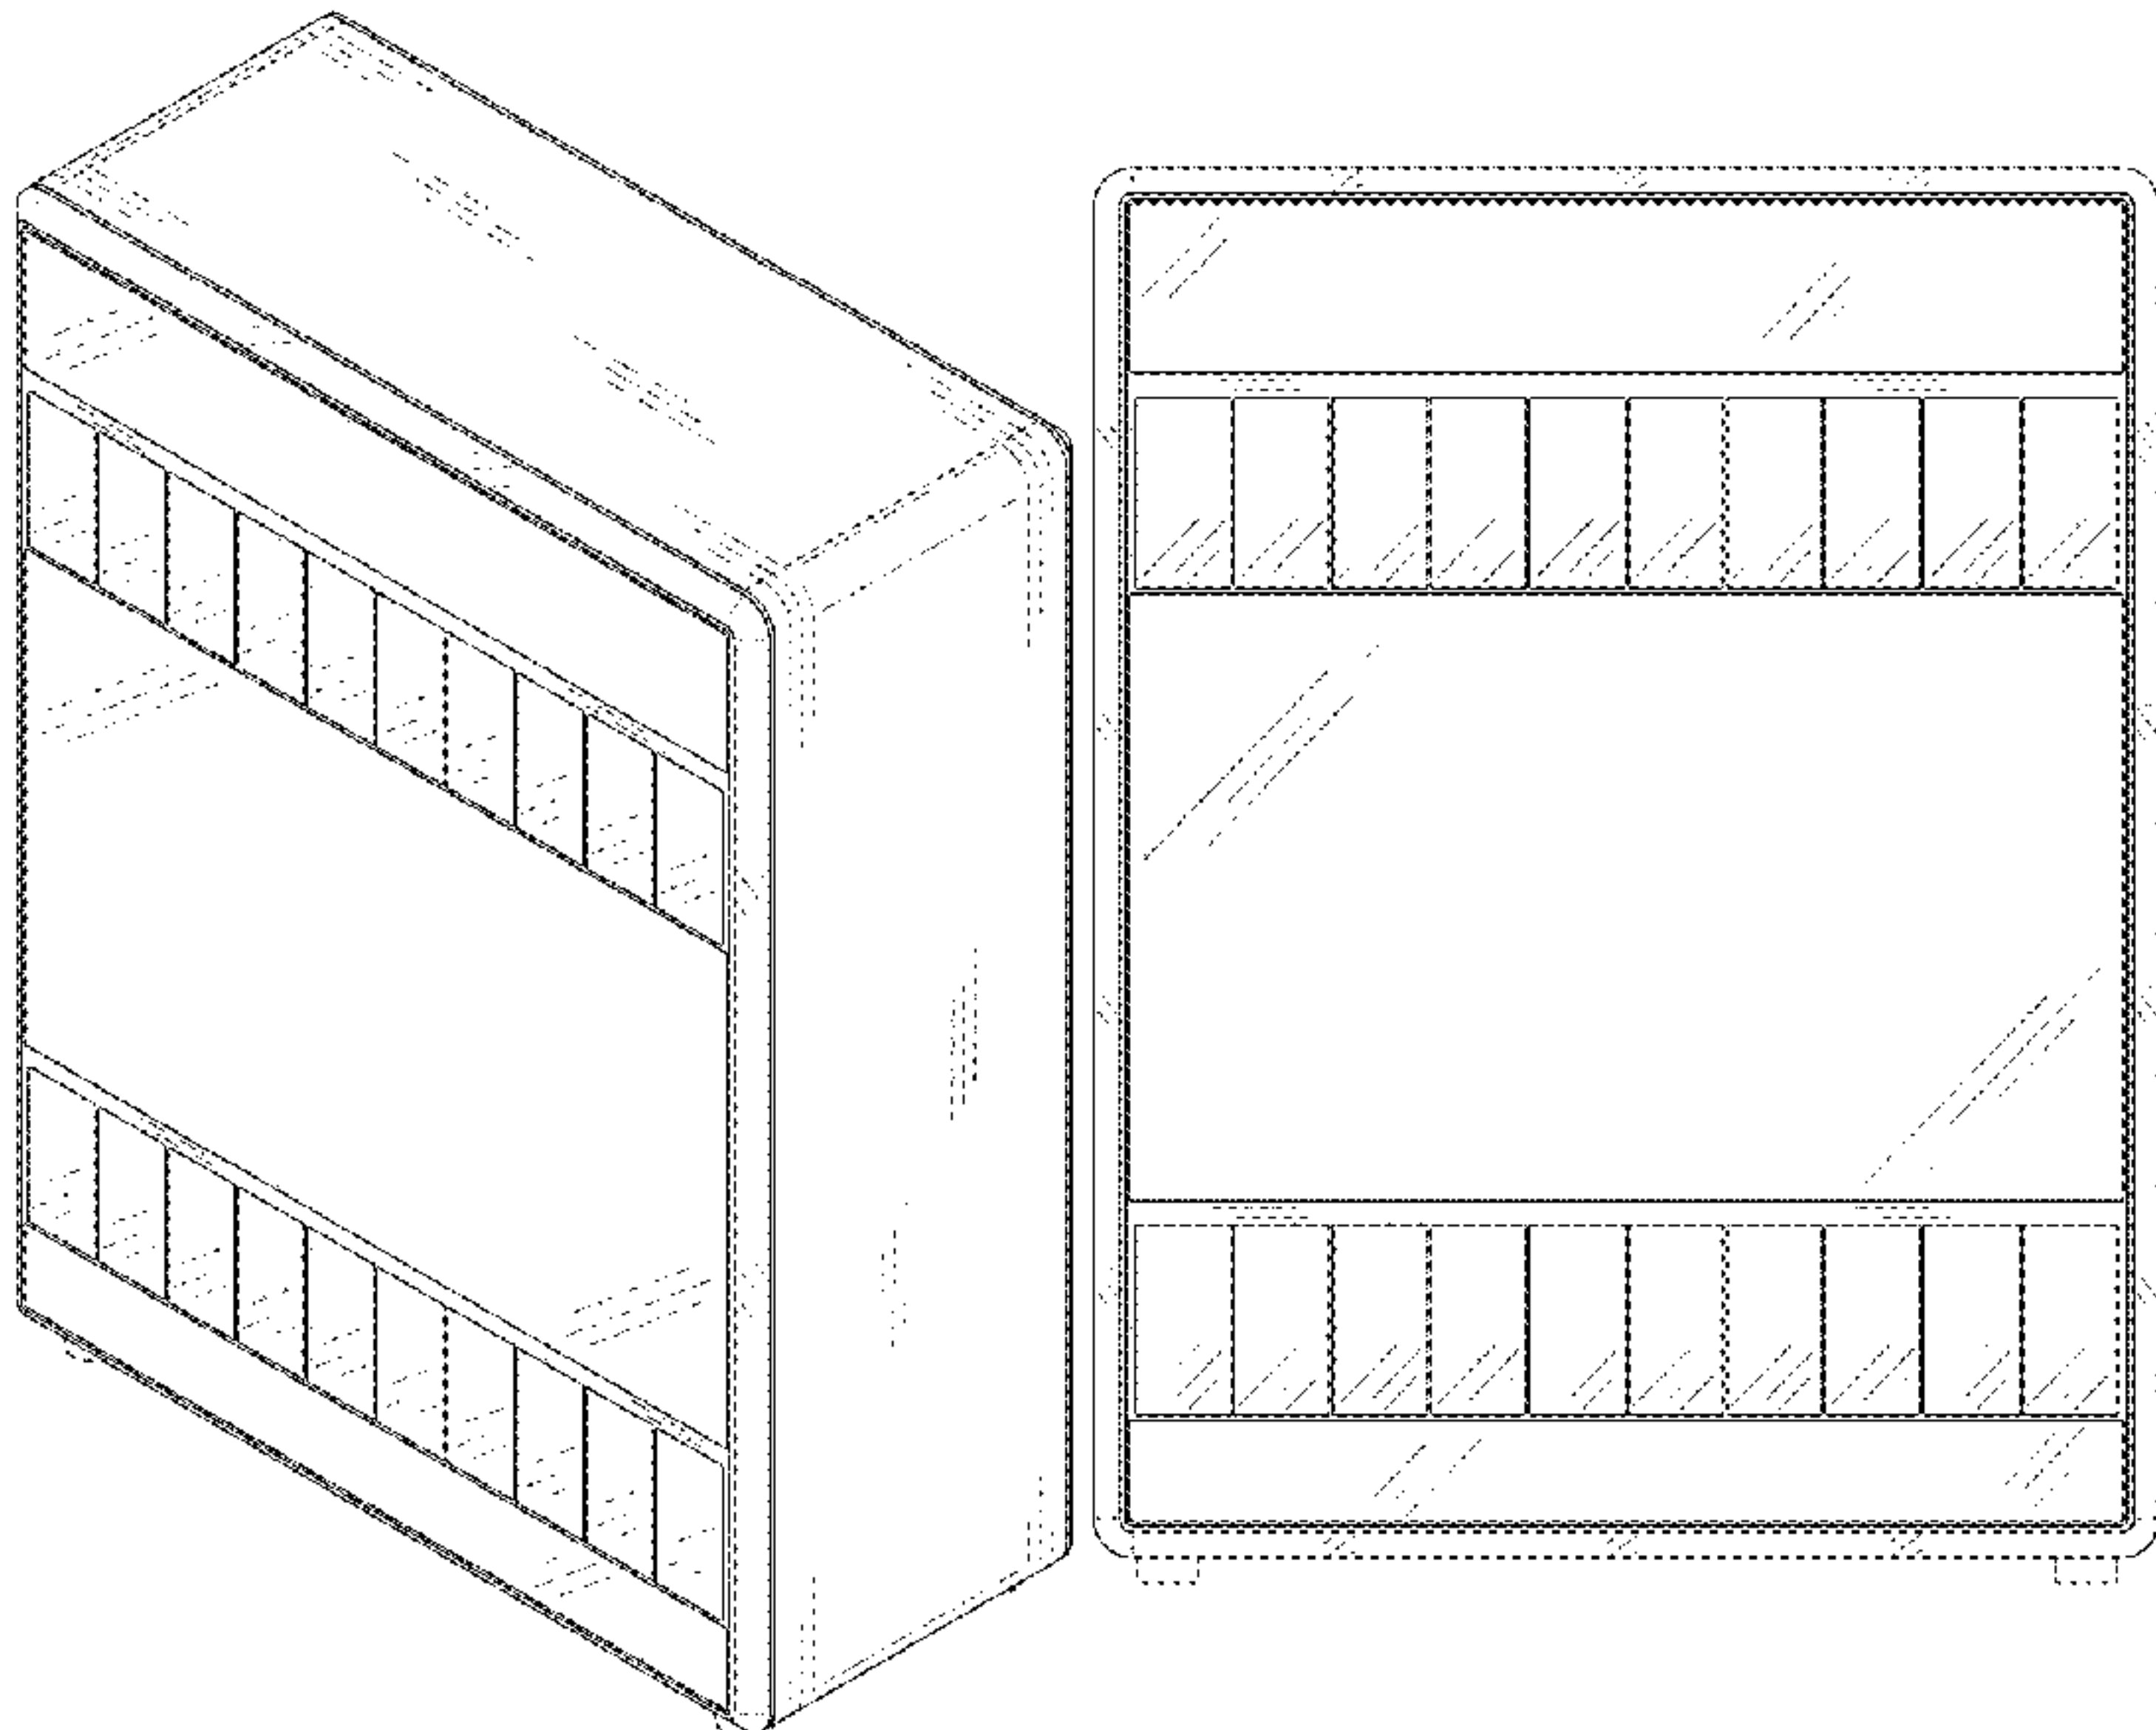

(56)

References Cited

U.S. PATENT DOCUMENTS

D774,659 S * 12/2016 Quackenbush D24/216
D785,198 S * 4/2017 Lemke D24/232
D796,749 S * 9/2017 Kessler D32/1
D800,000 S * 10/2017 Barton D24/216
D802,786 S * 11/2017 Chang D24/216
D804,049 S * 11/2017 Chang D24/216
D822,848 S * 7/2018 Lemke D24/232
D841,187 S * 2/2019 Kurz-Ottenwaelder D24/232
D843,597 S * 3/2019 Kurz-Ottenwaelder D24/232
D866,795 S * 11/2019 Sakai D24/232
D870,576 S * 12/2019 Kang D24/216
D878,625 S * 3/2020 Sakai D24/232
D879,994 S * 3/2020 Leimkuehler D24/216
D882,114 S * 4/2020 Erb D24/232
D883,510 S * 5/2020 Neuman D24/216
D884,996 S * 5/2020 Anselm D32/1
D885,216 S * 5/2020 Hu D24/232
D887,295 S * 6/2020 Carney D10/81
D887,296 S * 6/2020 Stone D24/216
D887,545 S * 6/2020 Heintze D24/107
D888,985 S * 6/2020 Hsieh D24/232
D890,357 S * 7/2020 Zanon D24/217
D891,278 S * 7/2020 Querrey D10/81
D896,981 S * 9/2020 Gruen D24/232
D897,874 S * 10/2020 Carney D10/81
D900,331 S * 10/2020 Livingston D24/216
D907,245 S * 1/2021 Rateike D24/232
D908,238 S * 1/2021 Cavada, Jr. D24/217

D911,546 S * 2/2021 Vacic D24/216
D914,231 S * 3/2021 Ong D24/216
D917,063 S * 4/2021 Ong D24/216
D918,418 S * 5/2021 Apotheloz D24/232
D920,144 S * 5/2021 Livingston D24/216
D920,145 S * 5/2021 Livingston D24/216
D921,223 S * 6/2021 Apotheloz D24/232
D923,197 S * 6/2021 Allegoren D24/232
D923,199 S * 6/2021 Luther D24/233
D930,181 S * 9/2021 Milliff D24/217
D931,118 S * 9/2021 Lee D24/232
D937,433 S * 11/2021 Sugie D24/158
D941,488 S * 1/2022 Fang D24/216
D944,472 S * 2/2022 Schmitt D32/1
D946,431 S * 3/2022 Blake D24/232
D954,288 S * 6/2022 Wade D24/216
D956,261 S * 6/2022 Segawa D24/232
D961,114 S * 8/2022 Kang D24/231
D967,456 S * 10/2022 Allegoren D24/232
D968,645 S * 11/2022 Allegoren D24/232
D978,369 S * 2/2023 Chang D24/216
D978,370 S * 2/2023 Gut D24/216
D979,787 S * 2/2023 Gruen D24/216
D980,096 S * 3/2023 Jiang D10/81
D992,750 S * 7/2023 Blair D24/216
D992,751 S * 7/2023 Liu D24/216
D999,399 S * 9/2023 Long D24/216
2015/0119268 A1 * 4/2015 Bishop G01N 1/31
435/7.1
2021/0151313 A1 * 5/2021 Ueda H01J 49/24

* cited by examiner

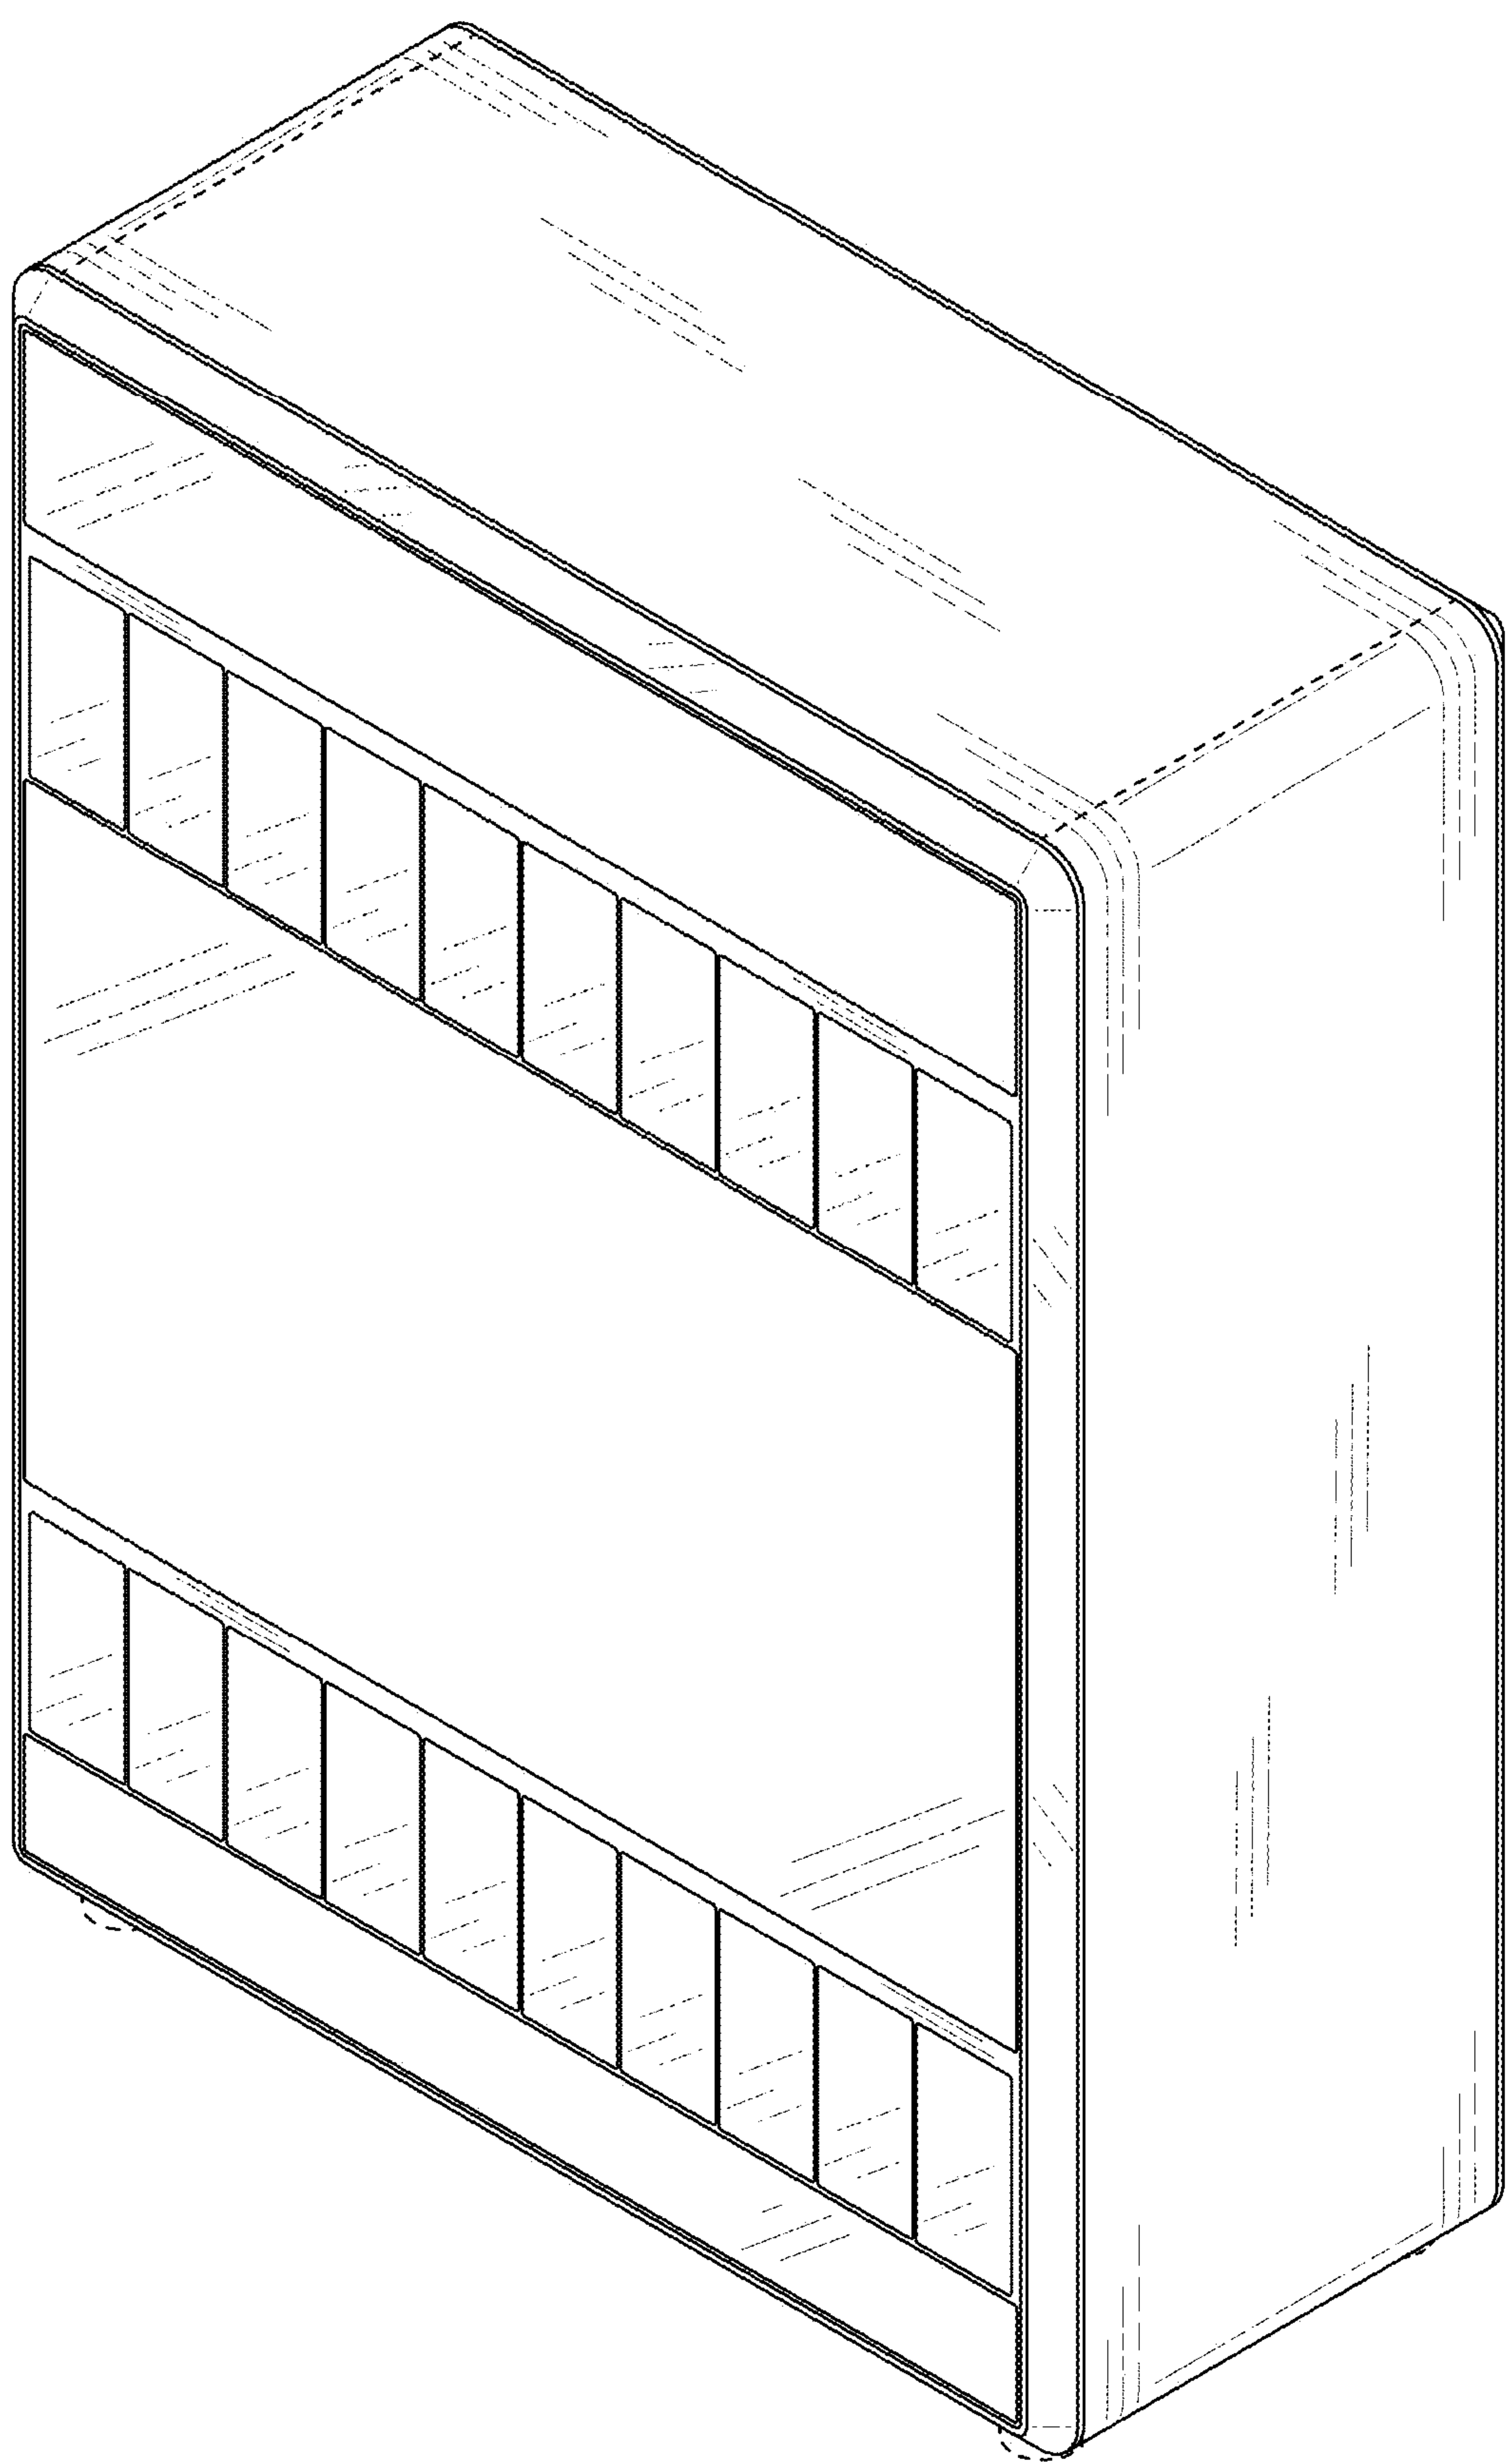


Figure 1

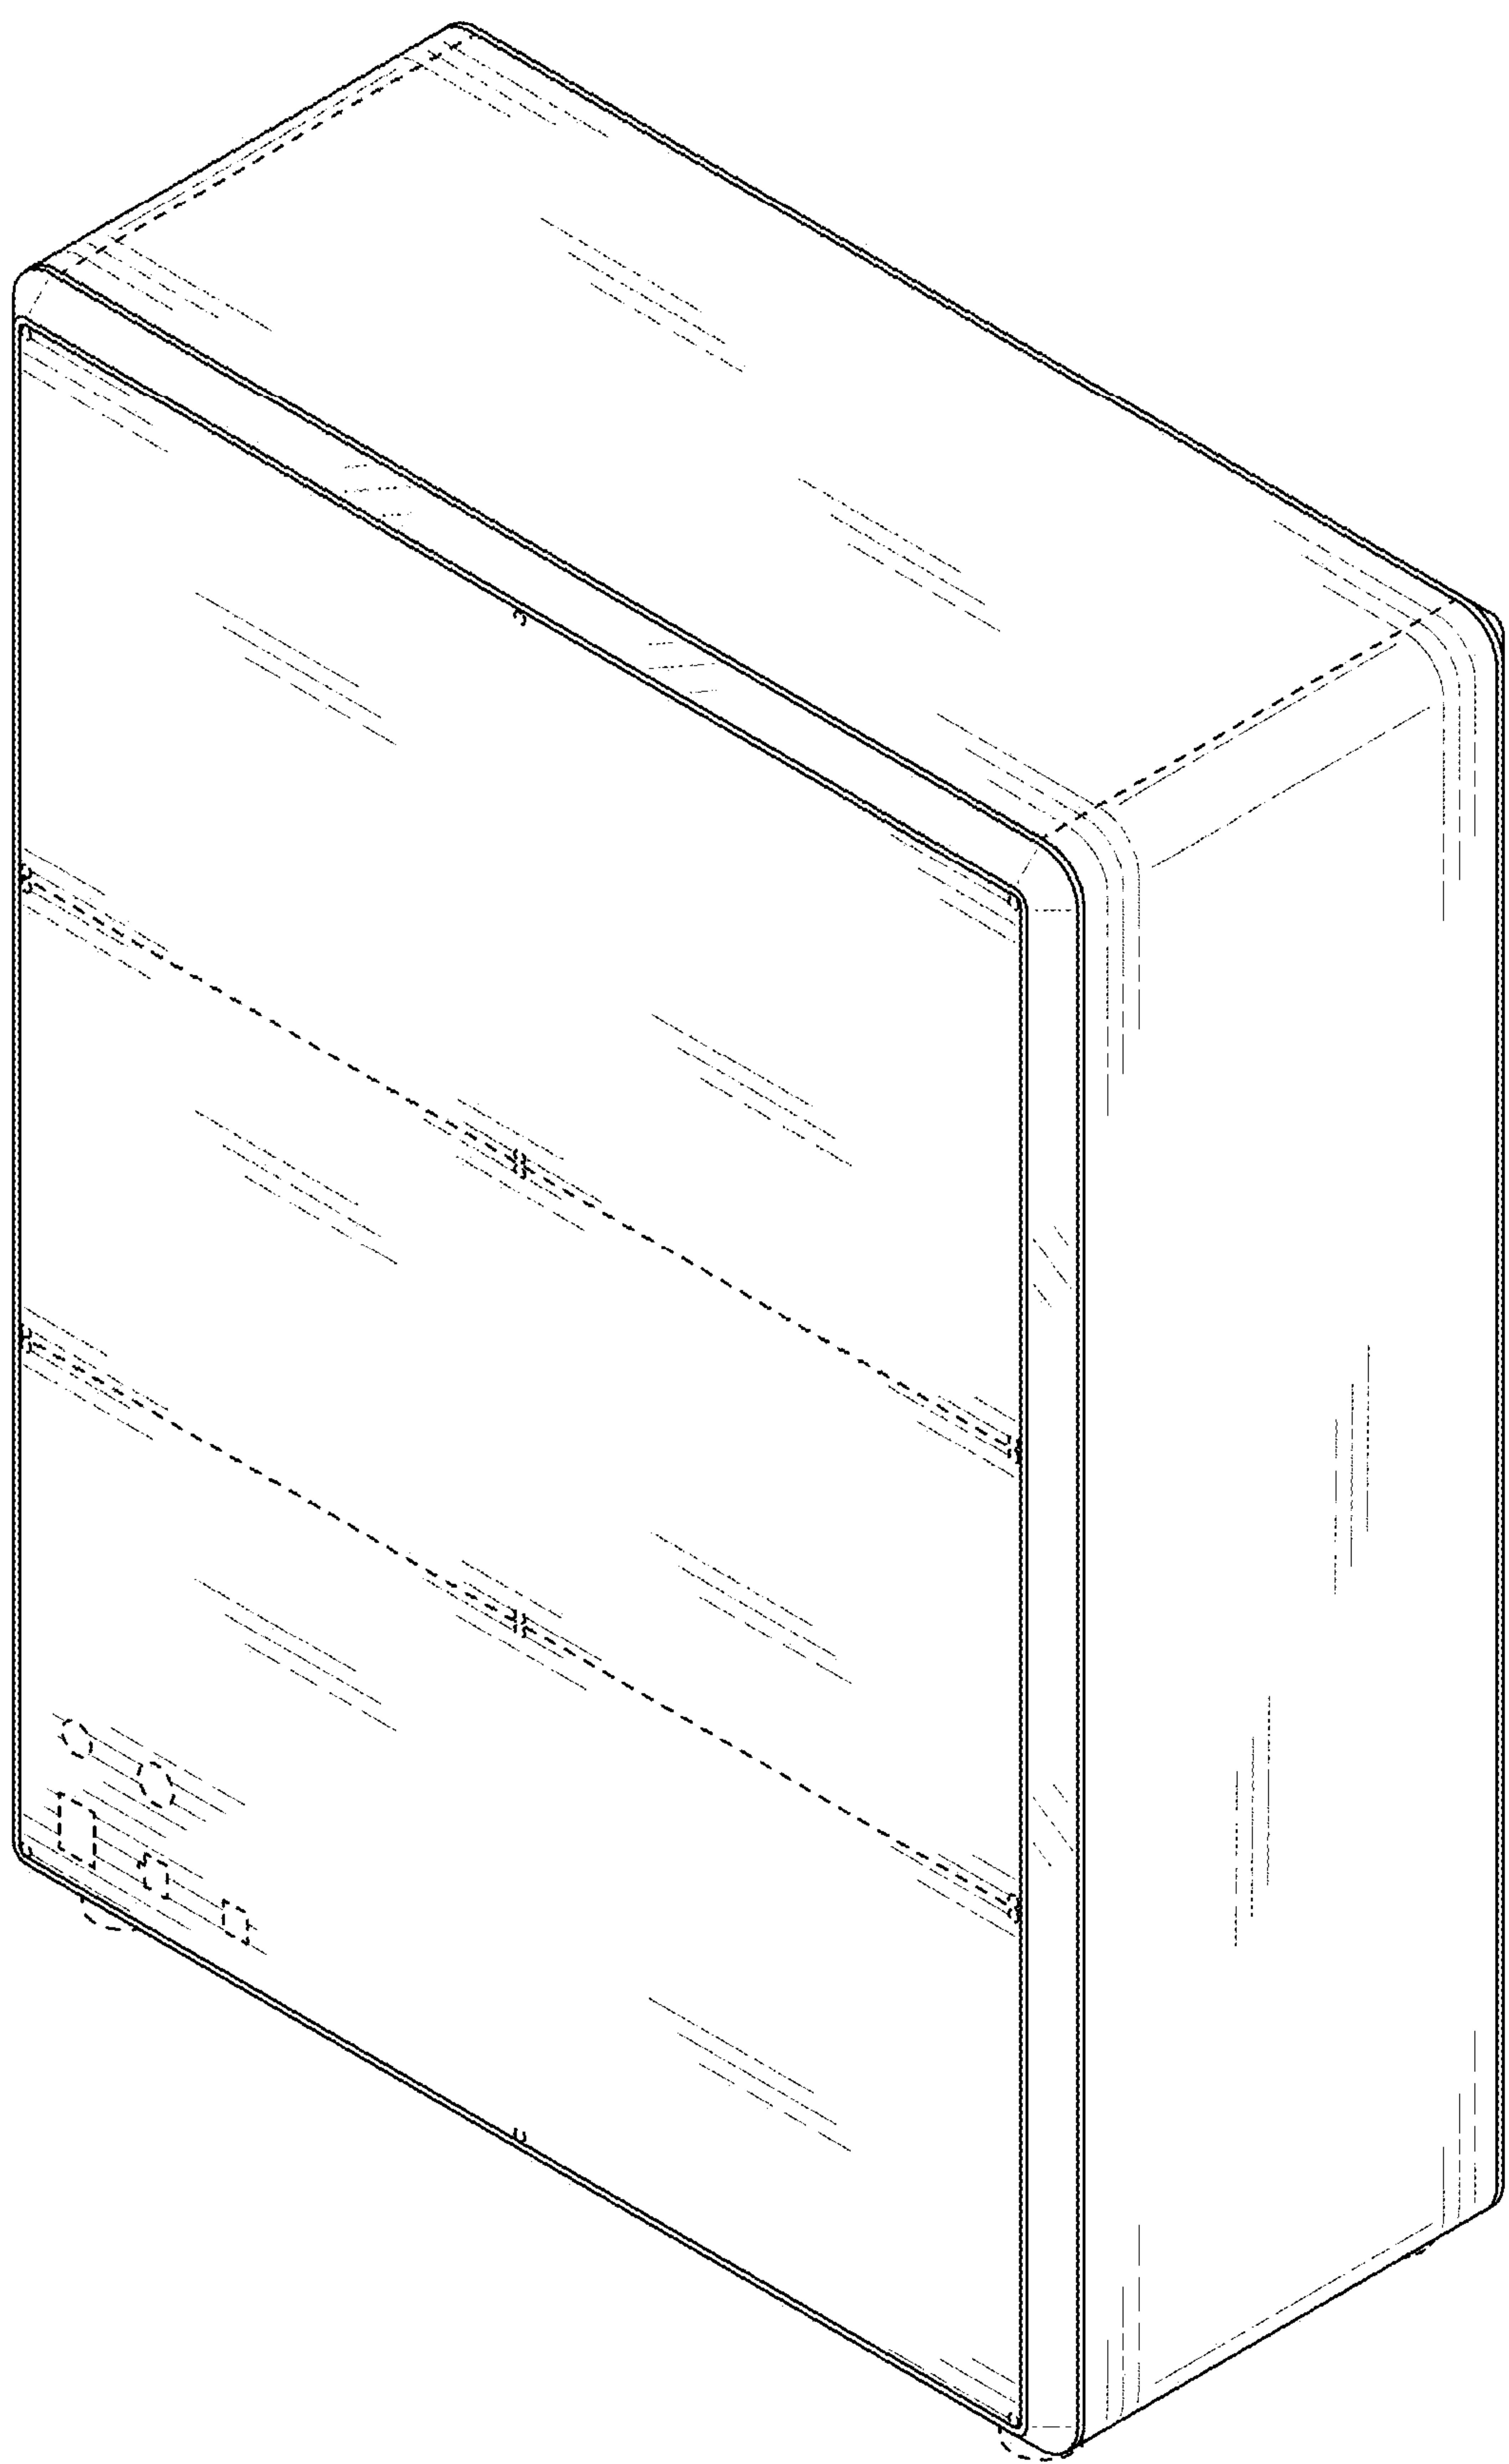


Figure 2



Figure 3

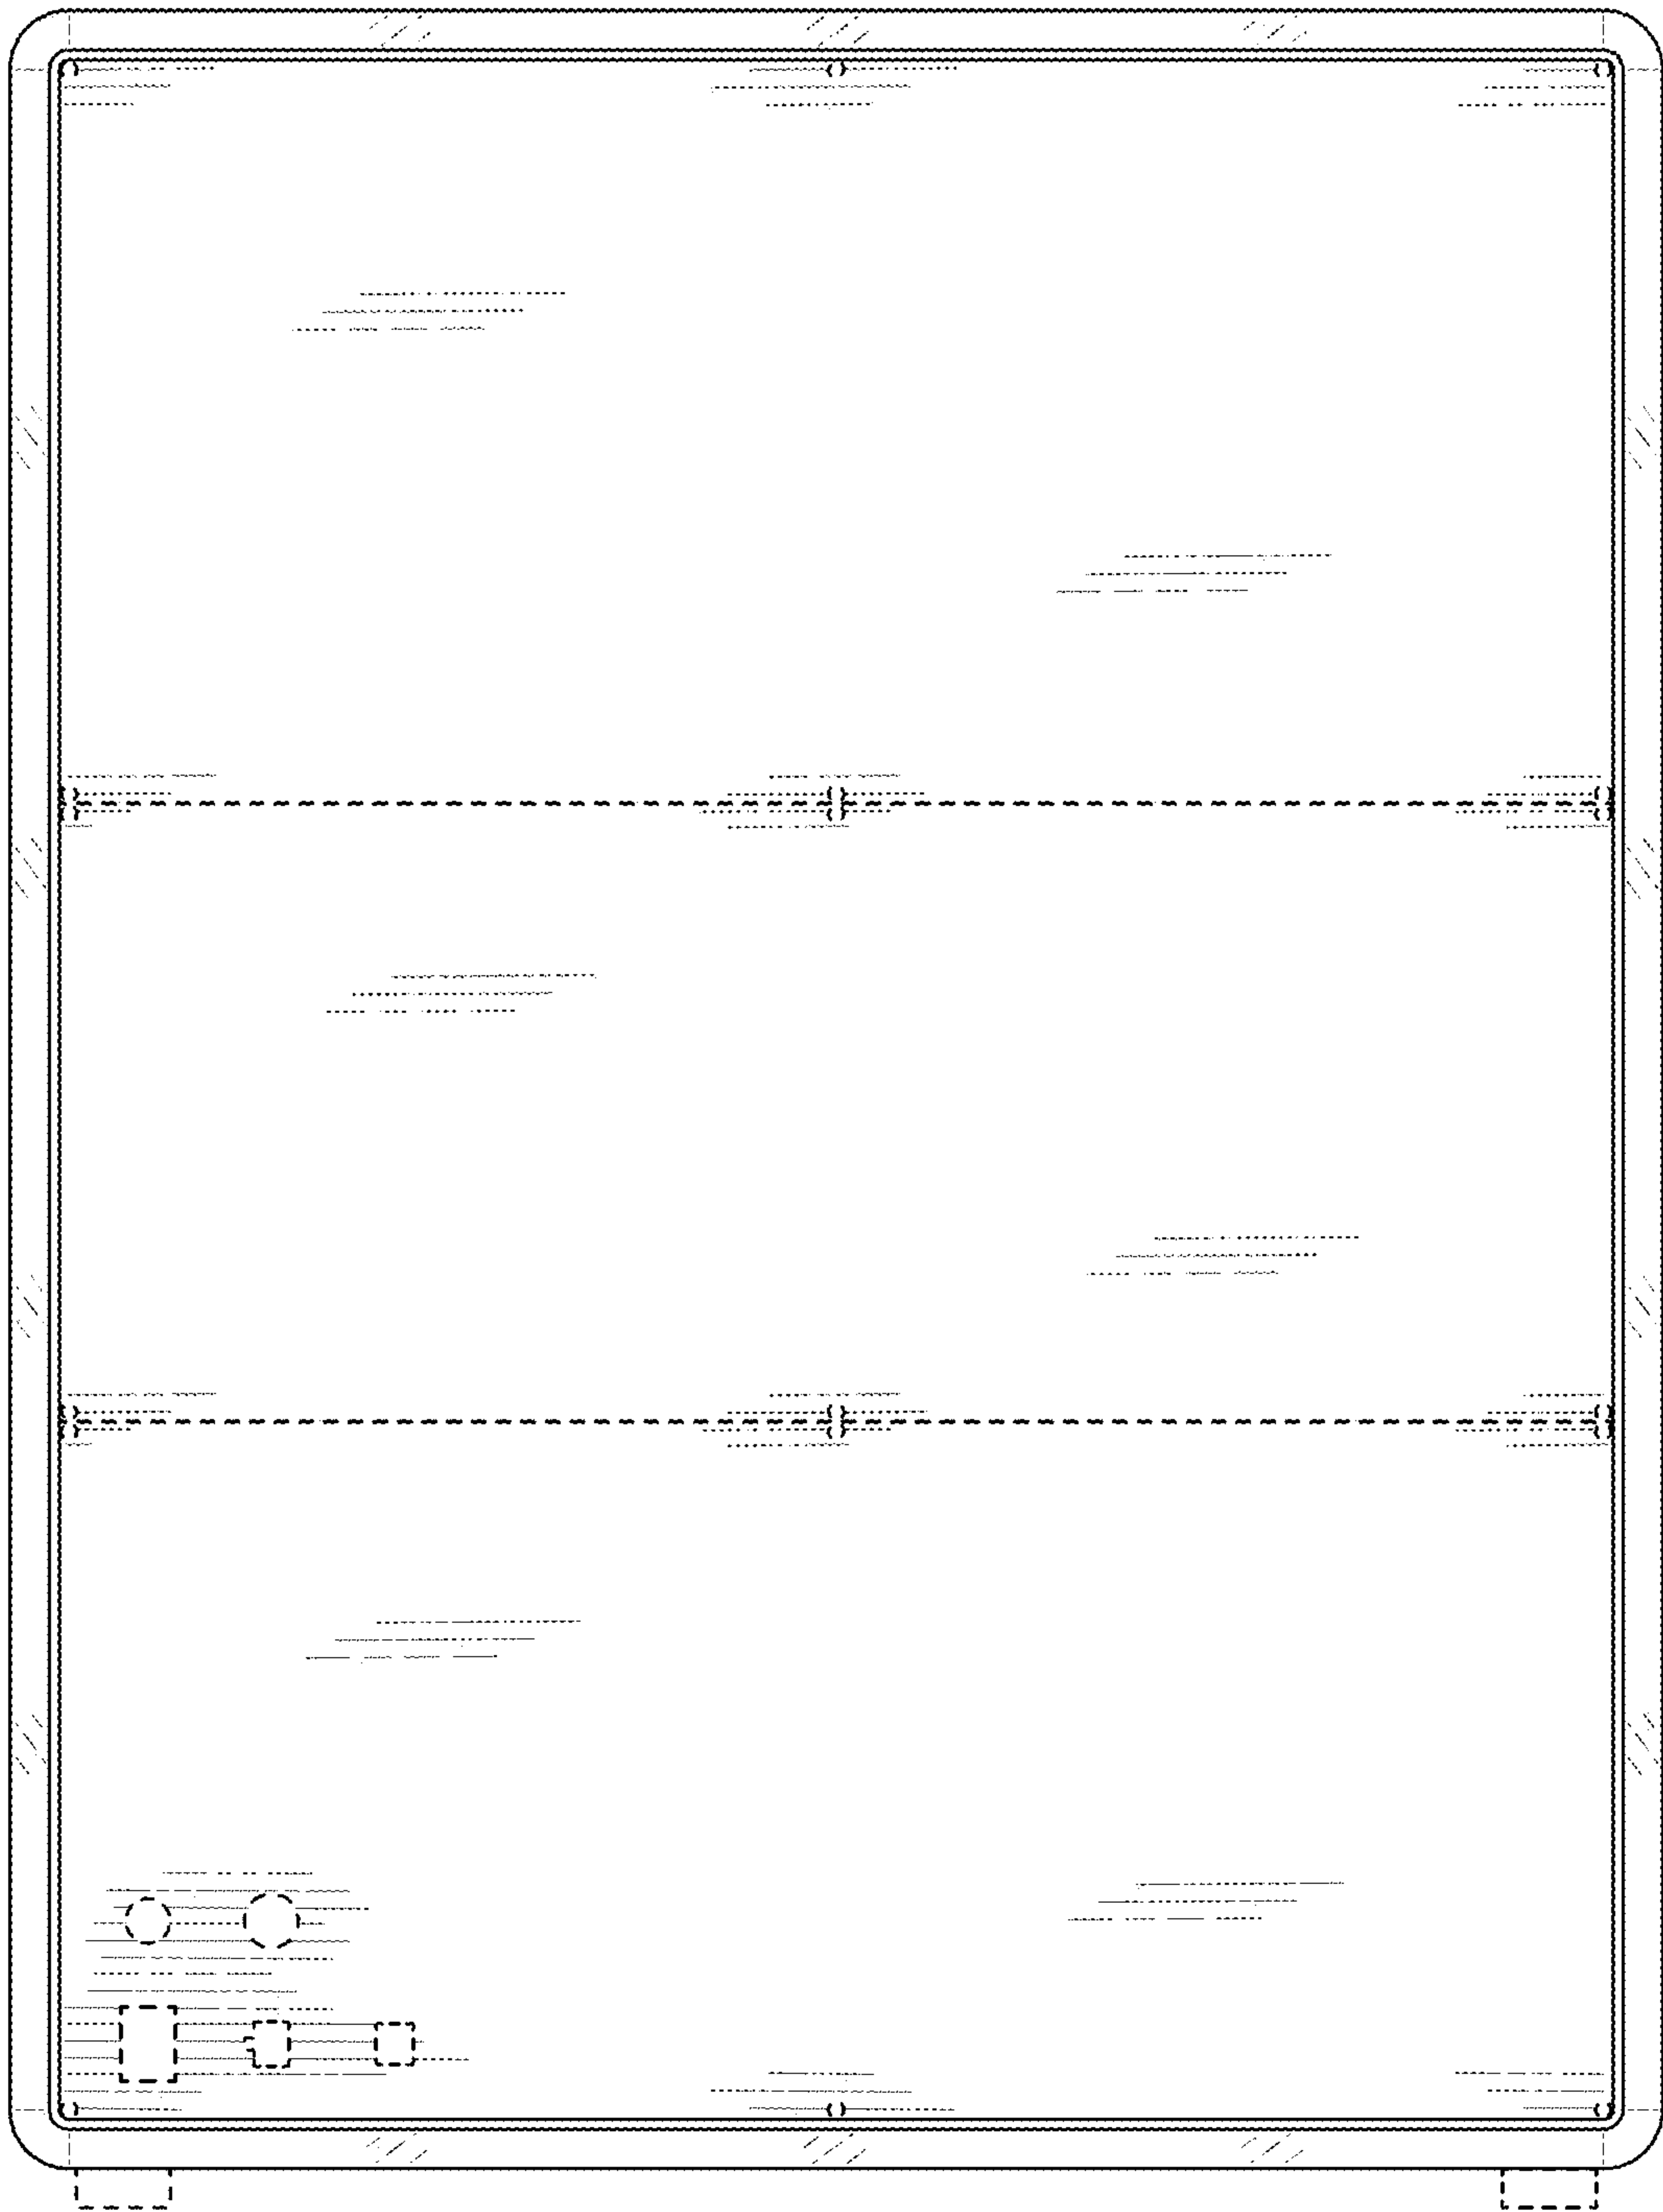


Figure 4

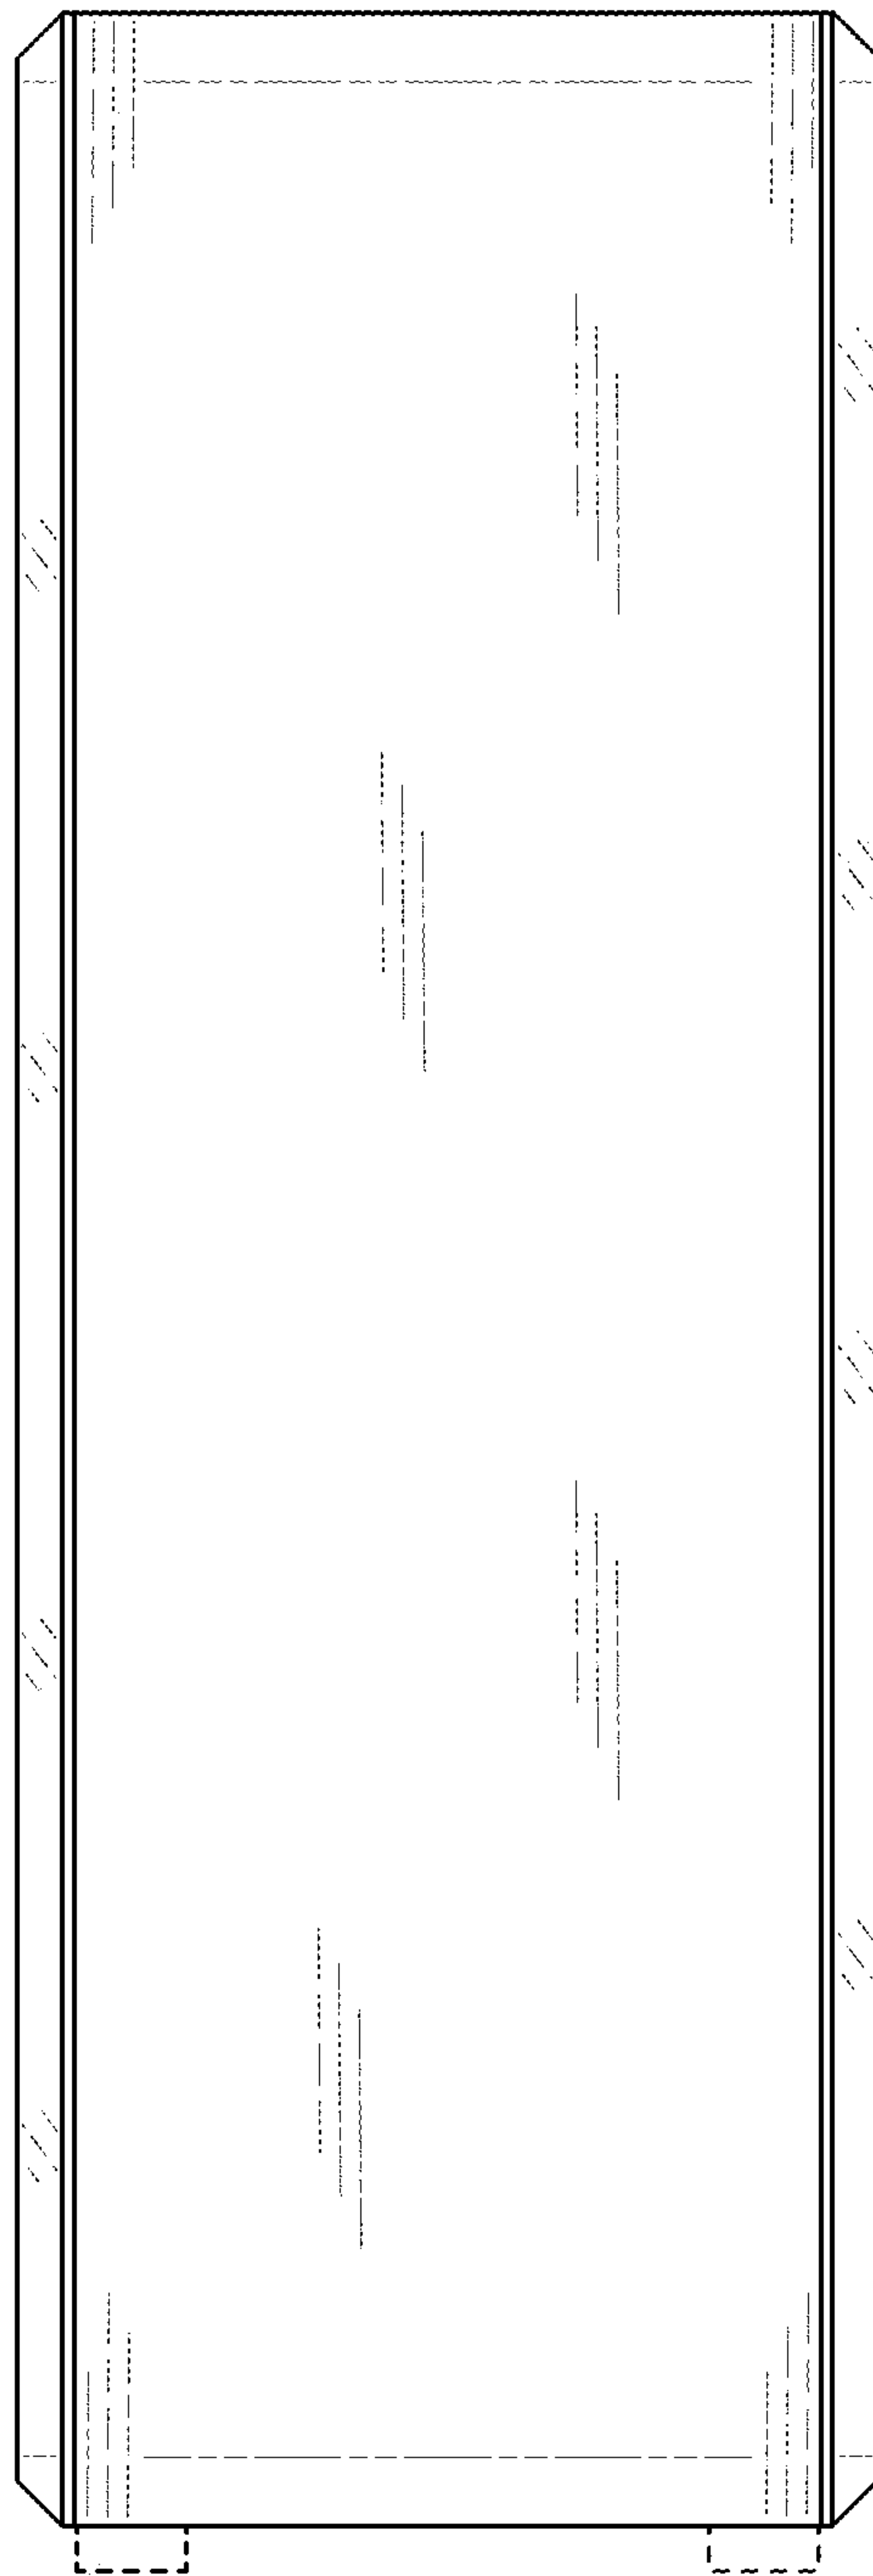


Figure 5

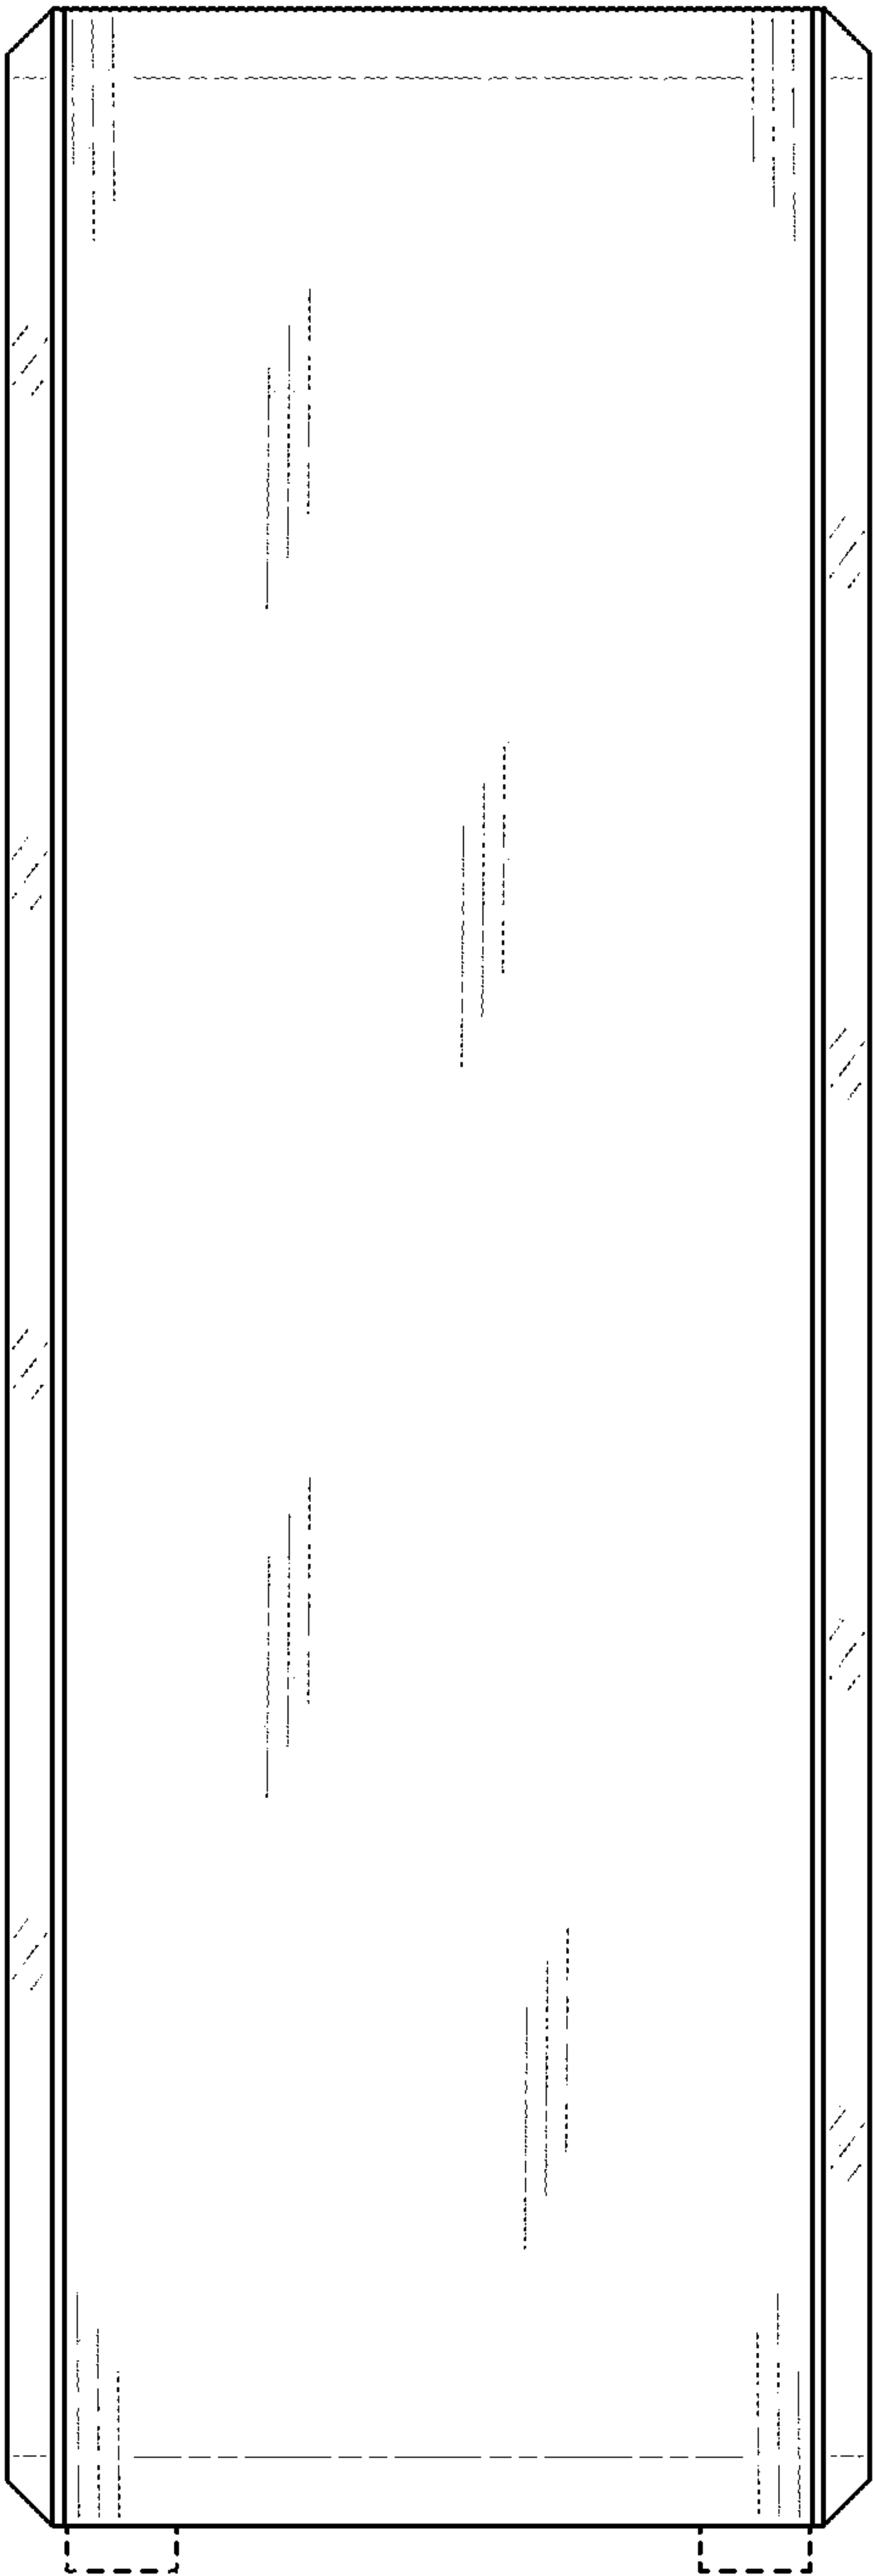


Figure 6

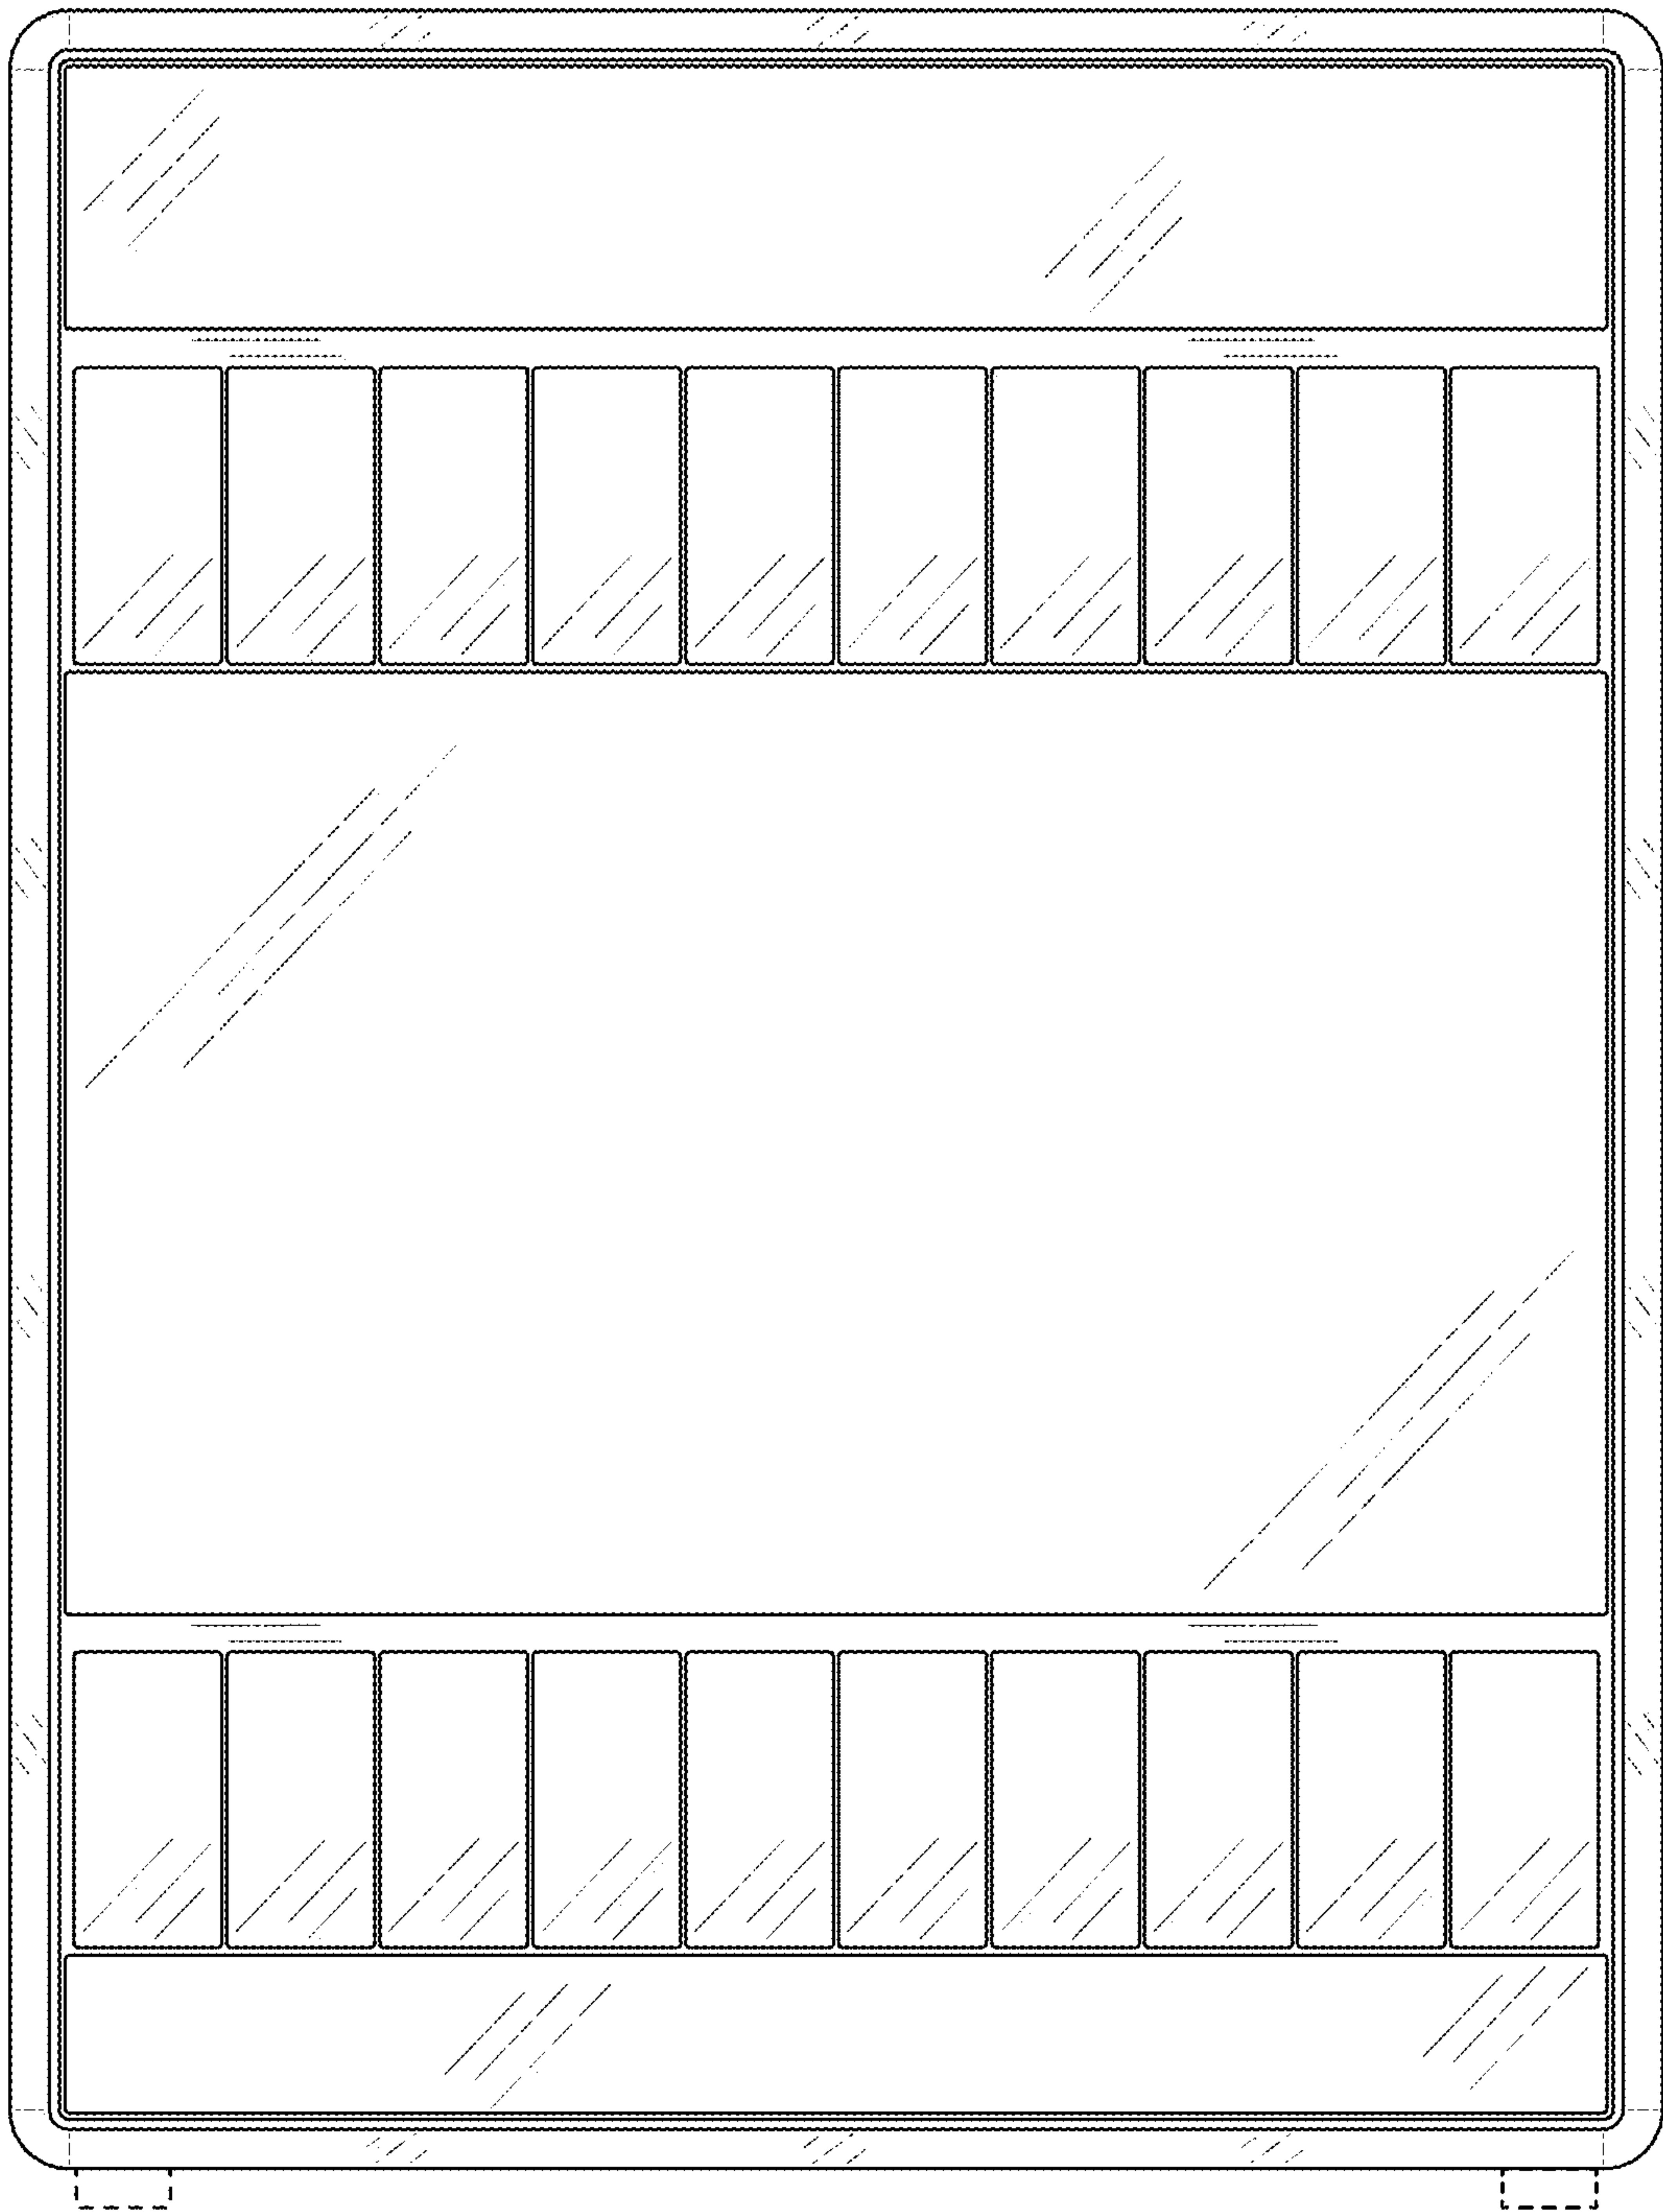


Figure 7



Figure 8