



US0D1027029S

(12)

United States Design Patent

Charlton et al.

(10) Patent No.:

US D1,027,029 S

(45) Date of Patent:

** *May 14, 2024

(54) PISTON AND LIGHTED RATE MONITOR

(71) Applicant: Prestan Products LLC, Mayfield Village, OH (US)

(72) Inventors: Christopher M Charlton, Mint Hill, NC (US); Mark E Cook, Stow, OH (US); Timothy E Lint, North Royalton, OH (US)

(73) Assignee: Prestan Products LLC, Mayfield Village, OH (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: 15 Years

(21) Appl. No.: 29/707,417

(22) Filed: Sep. 27, 2019

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. D24/167; D19/60

(58) Field of Classification Search USPC D19/59–64; D24/167

(Continued)

(56) References Cited

U.S. PATENT DOCUMENTS

4,850,876 A 7/1989 Lutaenko et al.
5,885,084 A 3/1999 Pastrick et al.
(Continued)

FOREIGN PATENT DOCUMENTS

CN 305343841 * 9/2019
JP D1073207 * 6/2000
(Continued)

OTHER PUBLICATIONS

Aedsuperstore. Link: <https://www.aedsuperstore.com/prestan-rpp-ulpistonm-1-ms-ultralite-adult-manikin-replacement-single-piston-with-cpr-feedback.html>, Visited Jul. 28, 2023. Prestan Ultralite Manikin w/CPR Feedback Replacement Piston (Year: 2023).*

(Continued)

Primary Examiner — Lauren D McVey
(74) Attorney, Agent, or Firm — FROST BROWN TODD LLP


(57) CLAIM

The ornamental design for a piston and lighted rate monitor, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a piston and lighted rate monitor in a use position in an environment;
FIG. 2 is a perspective top view thereof in a storage position without environment;
FIG. 3 is a perspective bottom view of the piston and lighted rate monitor of FIG. 2;
FIG. 4 is a top view of the piston and lighted rate monitor of FIG. 2;
FIG. 5 is a bottom view of the piston and lighted rate monitor of FIG. 2;
FIG. 6 is a bottom end view of the piston and lighted rate monitor of FIG. 2;
FIG. 7 is a top end view of the piston and lighted rate monitor of FIG. 2;
FIG. 8 is a left side view of the piston and lighted rate monitor of FIG. 2;
FIG. 9 is a right side view of the piston and lighted rate monitor of FIG. 2;
FIG. 10 is a perspective top view showing the piston and lighted rate monitor of FIG. 1 in position for use; and,
FIG. 11 is a perspective top view of the piston and lighted rate monitor of FIG. 10.
The broken lines are provided solely for illustrative purposes and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

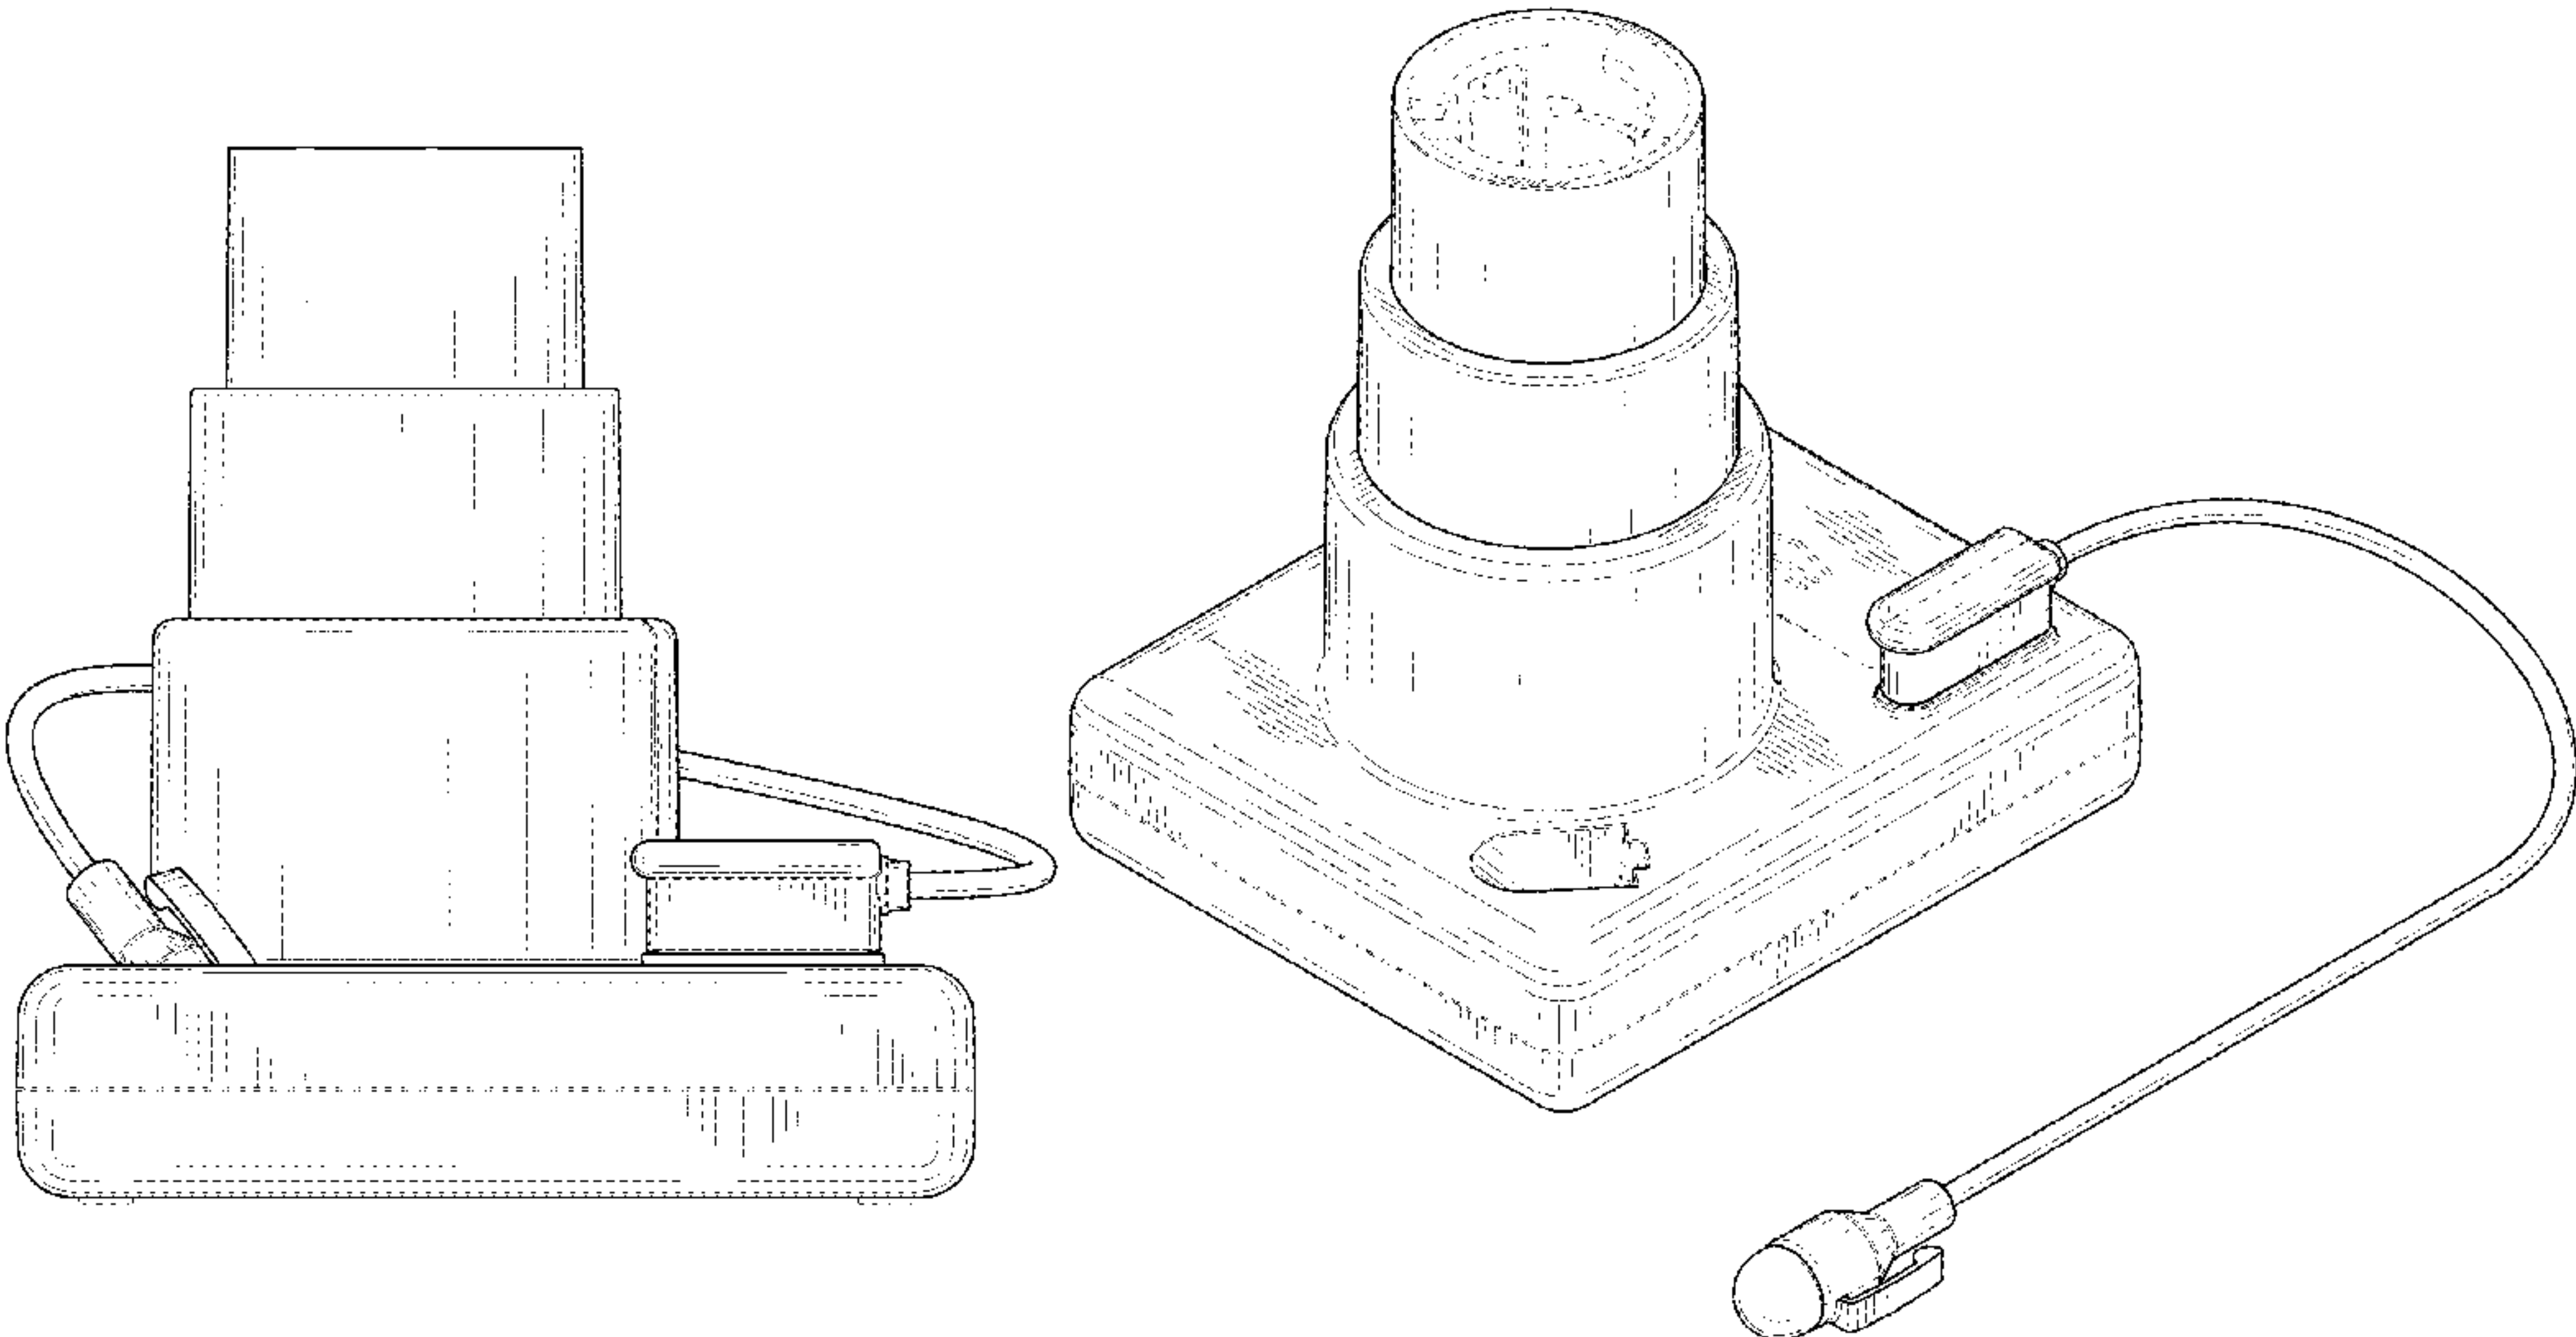

(58) **Field of Classification Search**
CPC A61H 31/00; A61H 31/004; A61H 31/005;
A61H 31/006; A61H 31/007; G09B
23/288
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS

8,465,293 B2 6/2013 Pastrick et al.
D718,867 S * 12/2014 Schroderus D24/167
9,092,995 B2 7/2015 Pastrick et al.
9,852,659 B2 12/2017 Pastrick et al.
9,881,521 B2 * 1/2018 Pastrick G09B 23/28
10,269,267 B2 4/2019 Chung et al.
10,665,131 B2 * 5/2020 Olmstead G09B 23/288
D909,584 S * 2/2021 Kalchman D24/167
2005/0058977 A1 3/2005 Cantrell et al.
2007/0054254 A1 3/2007 Cook et al.
2007/0264621 A1 11/2007 Nysaether et al.
2009/0035740 A1 2/2009 Reed et al.
2010/0021876 A1 1/2010 Clash
2011/0091852 A1 * 4/2011 Stahler G09B 23/288
434/262
2013/0292319 A1 * 11/2013 Fulkerson A61M 1/16
210/321.78
2014/0342332 A1 * 11/2014 Olmstead G09B 23/288
434/266

2015/0079567 A1 * 3/2015 Mansi G09B 23/288
434/265
2016/0158097 A1 * 6/2016 Harper A61F 5/56
601/48
2016/0335921 A1 11/2016 Chung et al.
2017/0372639 A1 * 12/2017 Cowperthwait G09B 23/285
2022/0117471 A1 * 4/2022 Antonioli A61B 1/00006
2022/0277669 A1 * 9/2022 Charlton A61H 31/00
2023/0186788 A1 * 6/2023 Charlton G09B 5/02
434/265


FOREIGN PATENT DOCUMENTS

JP 2014533155 A * 12/2014 A61M 1/28
JP 7026645 B2 * 2/2022 A61B 1/00009
WO WO-2014105755 A1 * 7/2014 A61M 1/1039
WO 2021062344 A1 4/2021

OTHER PUBLICATIONS

Aedsuperstore. Link: https://www.aedsuperstore.com/prestan-products-professional-adult-manikin-replacement-monitor.html?select2=1&gclid=EAlaIQobChMI9qW2v--xgAMV5watBh2sqgySEAQYBiABEgIONvD_BwE , Visited Jul. 28, 2023. Prestan Monitor for the Professional Adult Manikin (Year: 2023).*

* cited by examiner

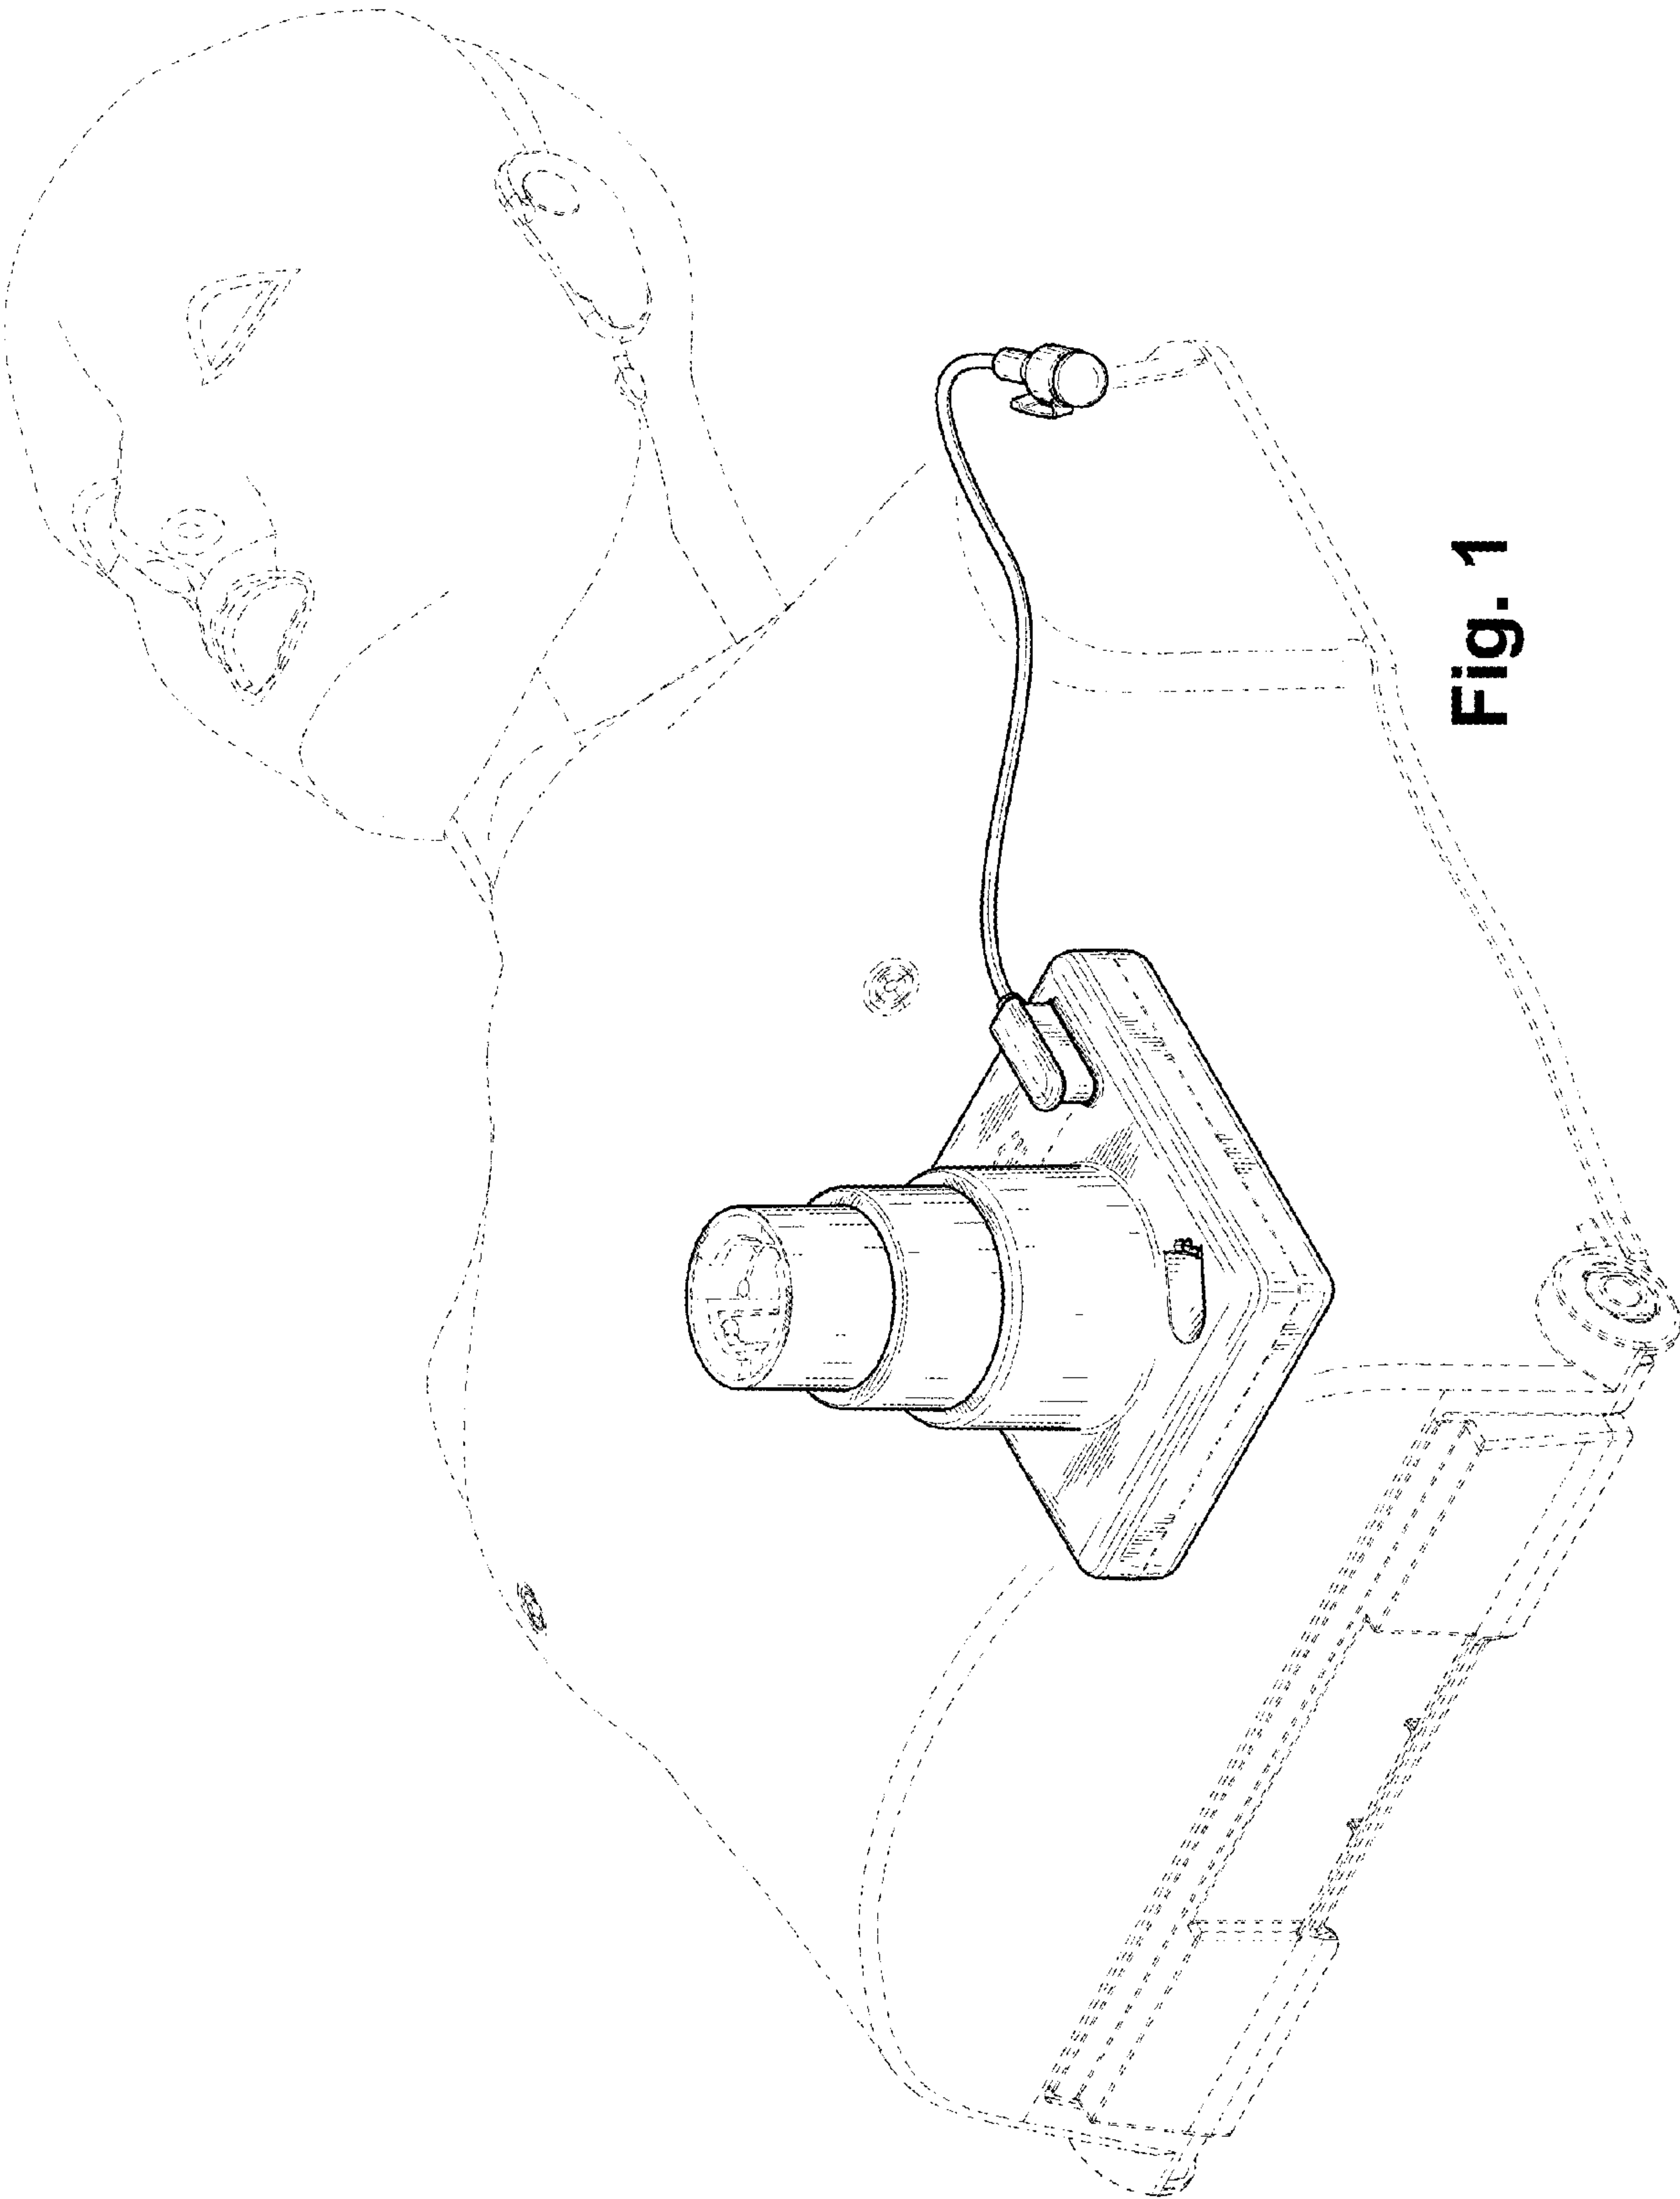

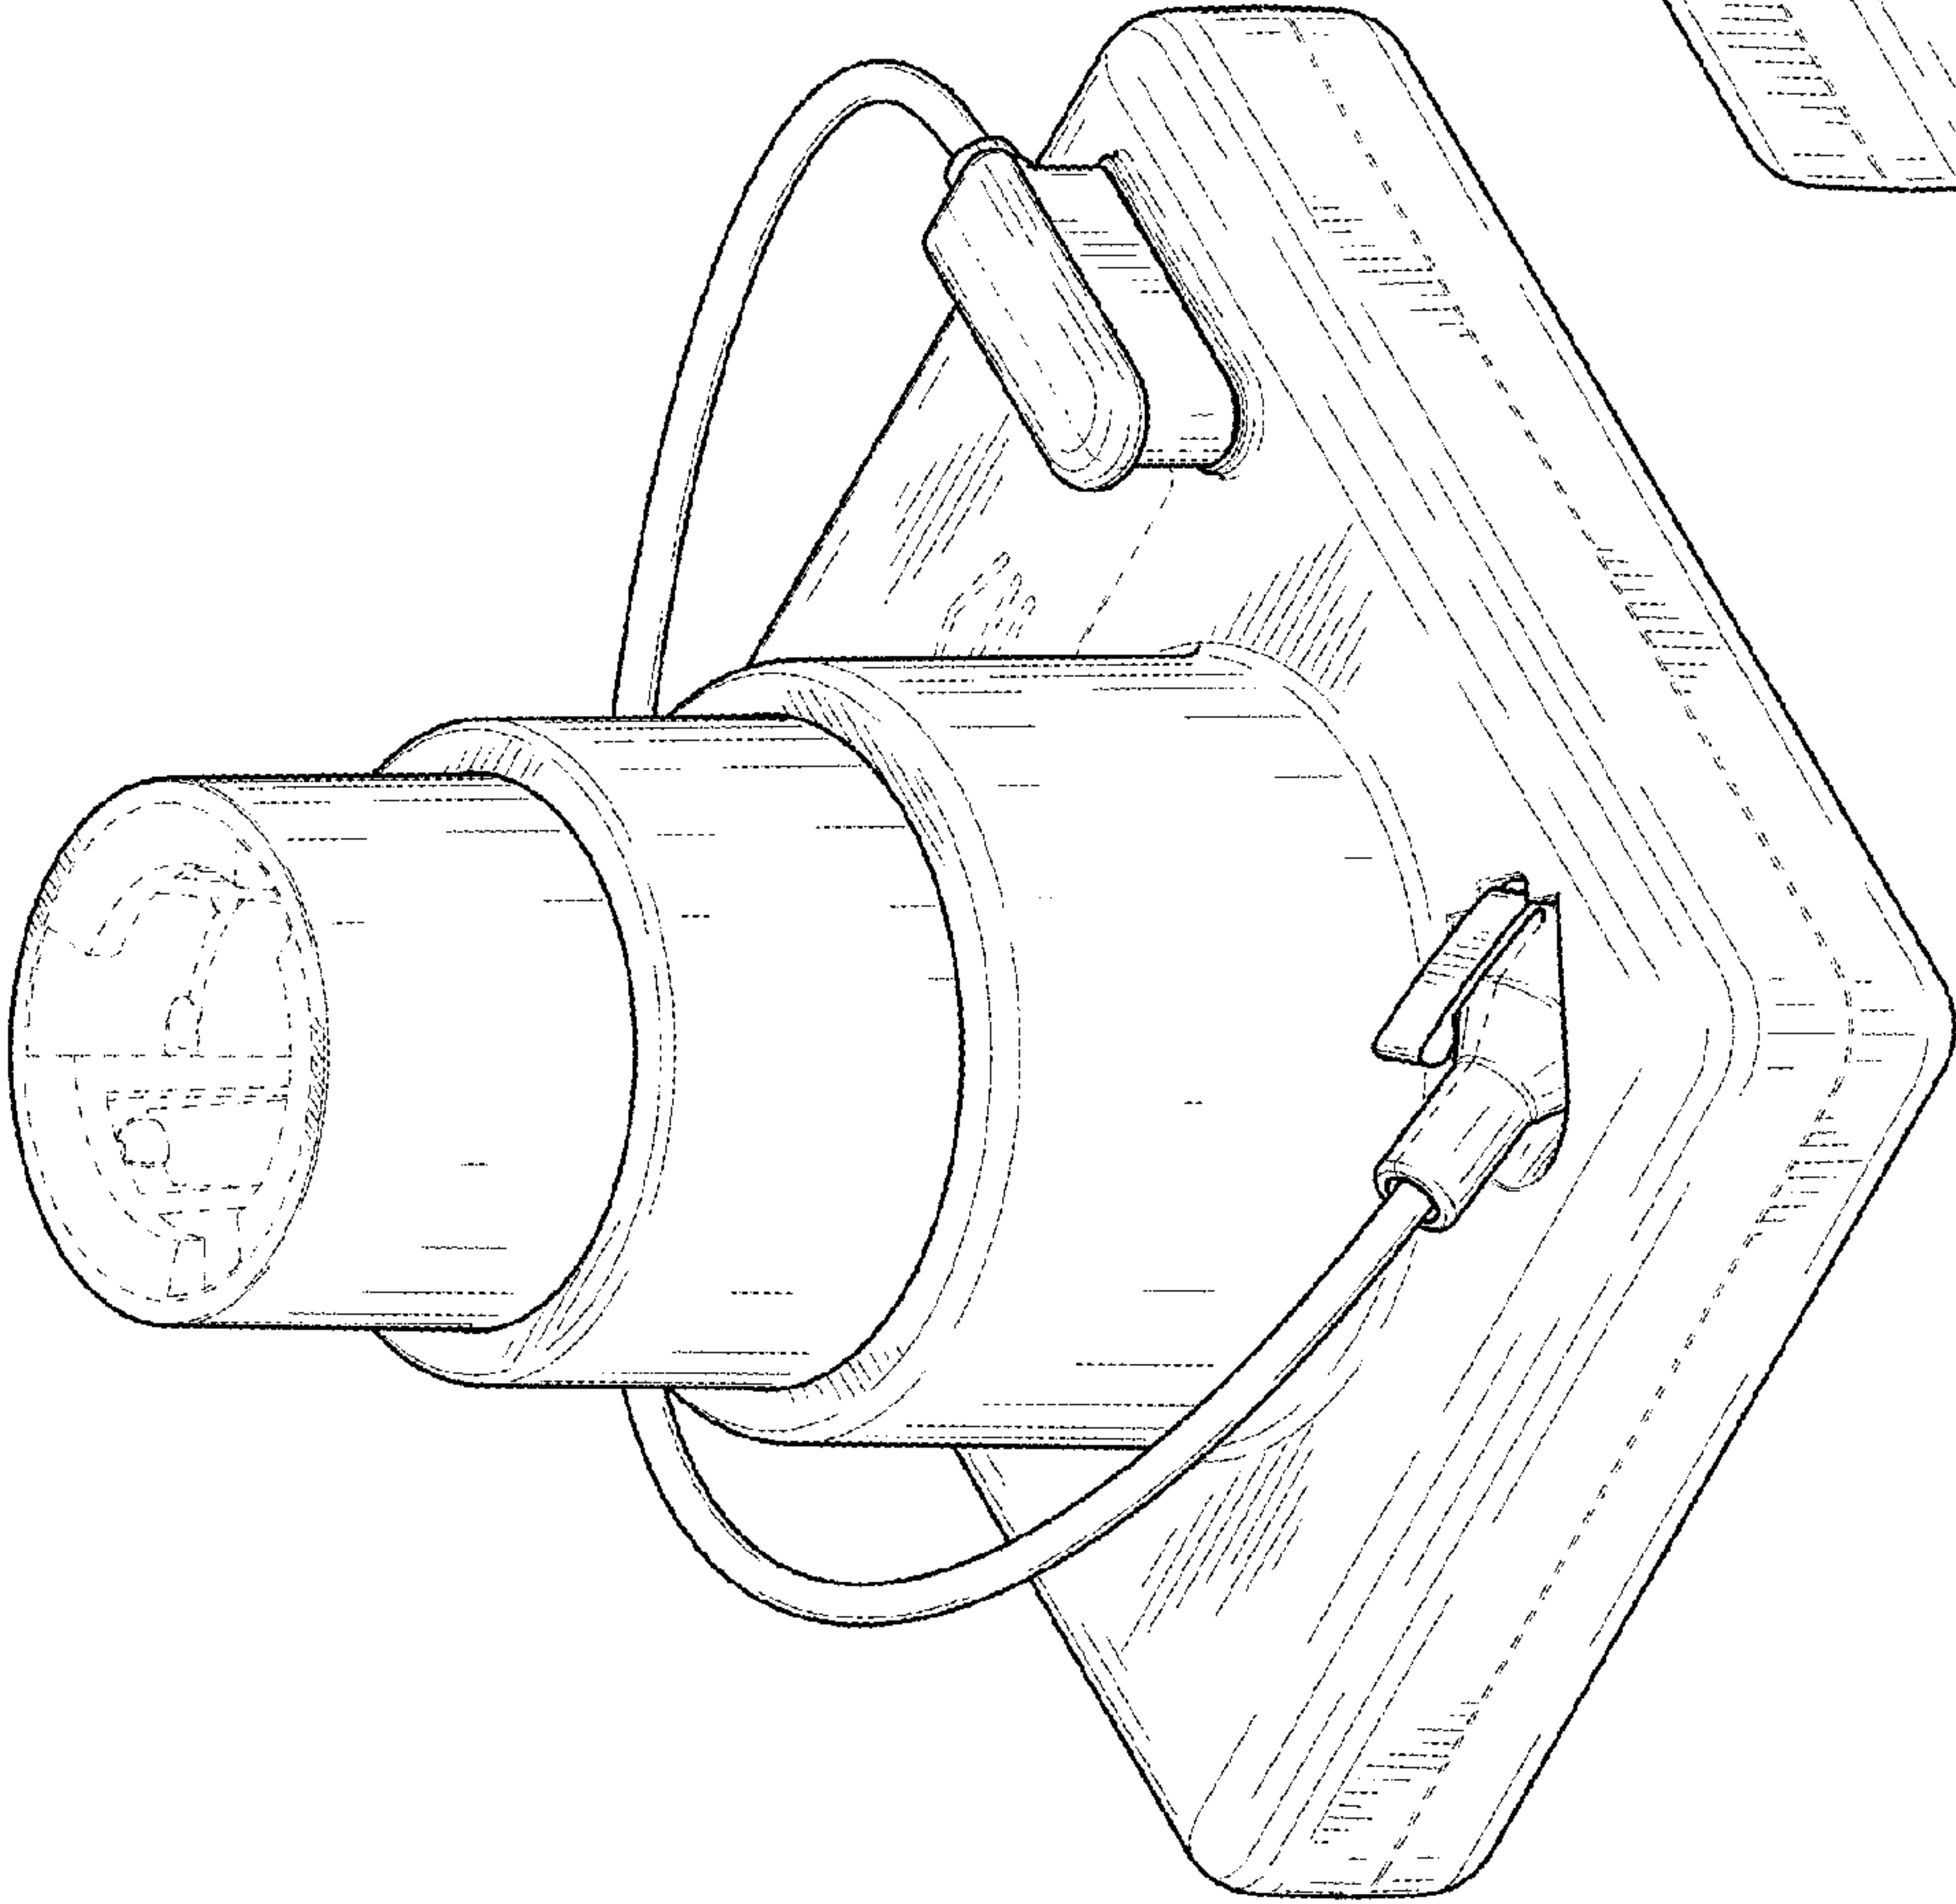


Fig. 2

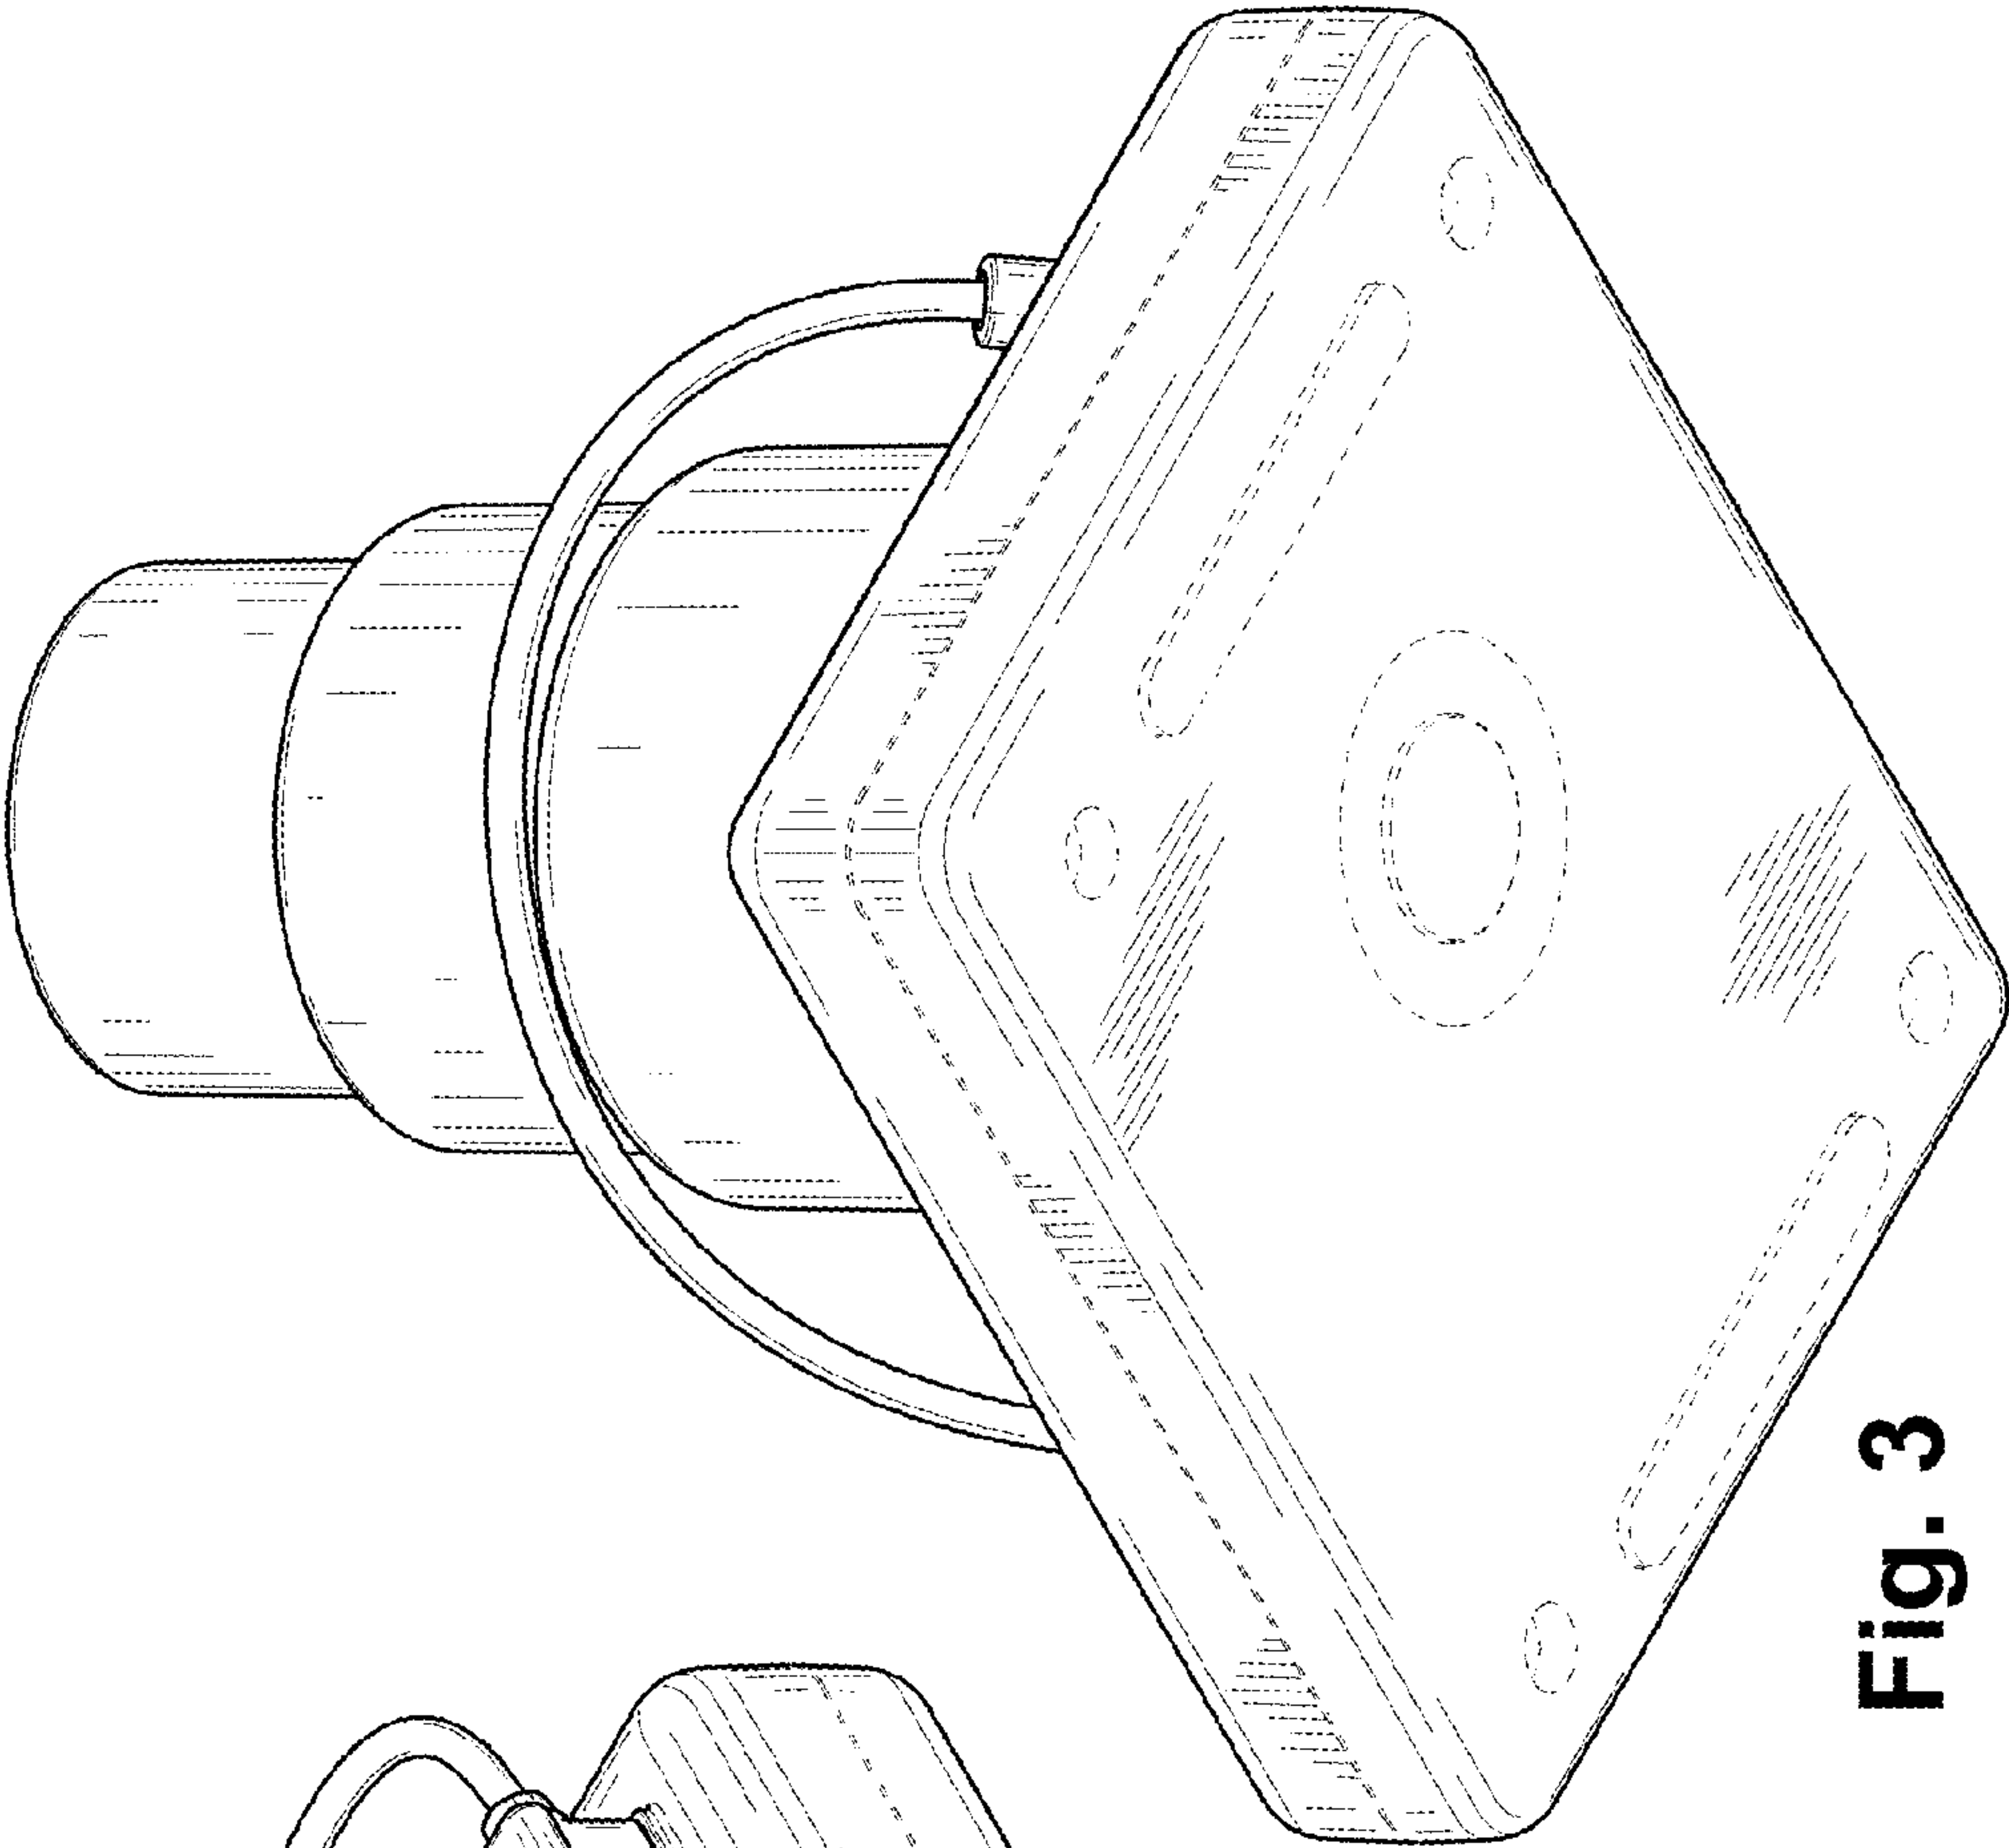


Fig. 3

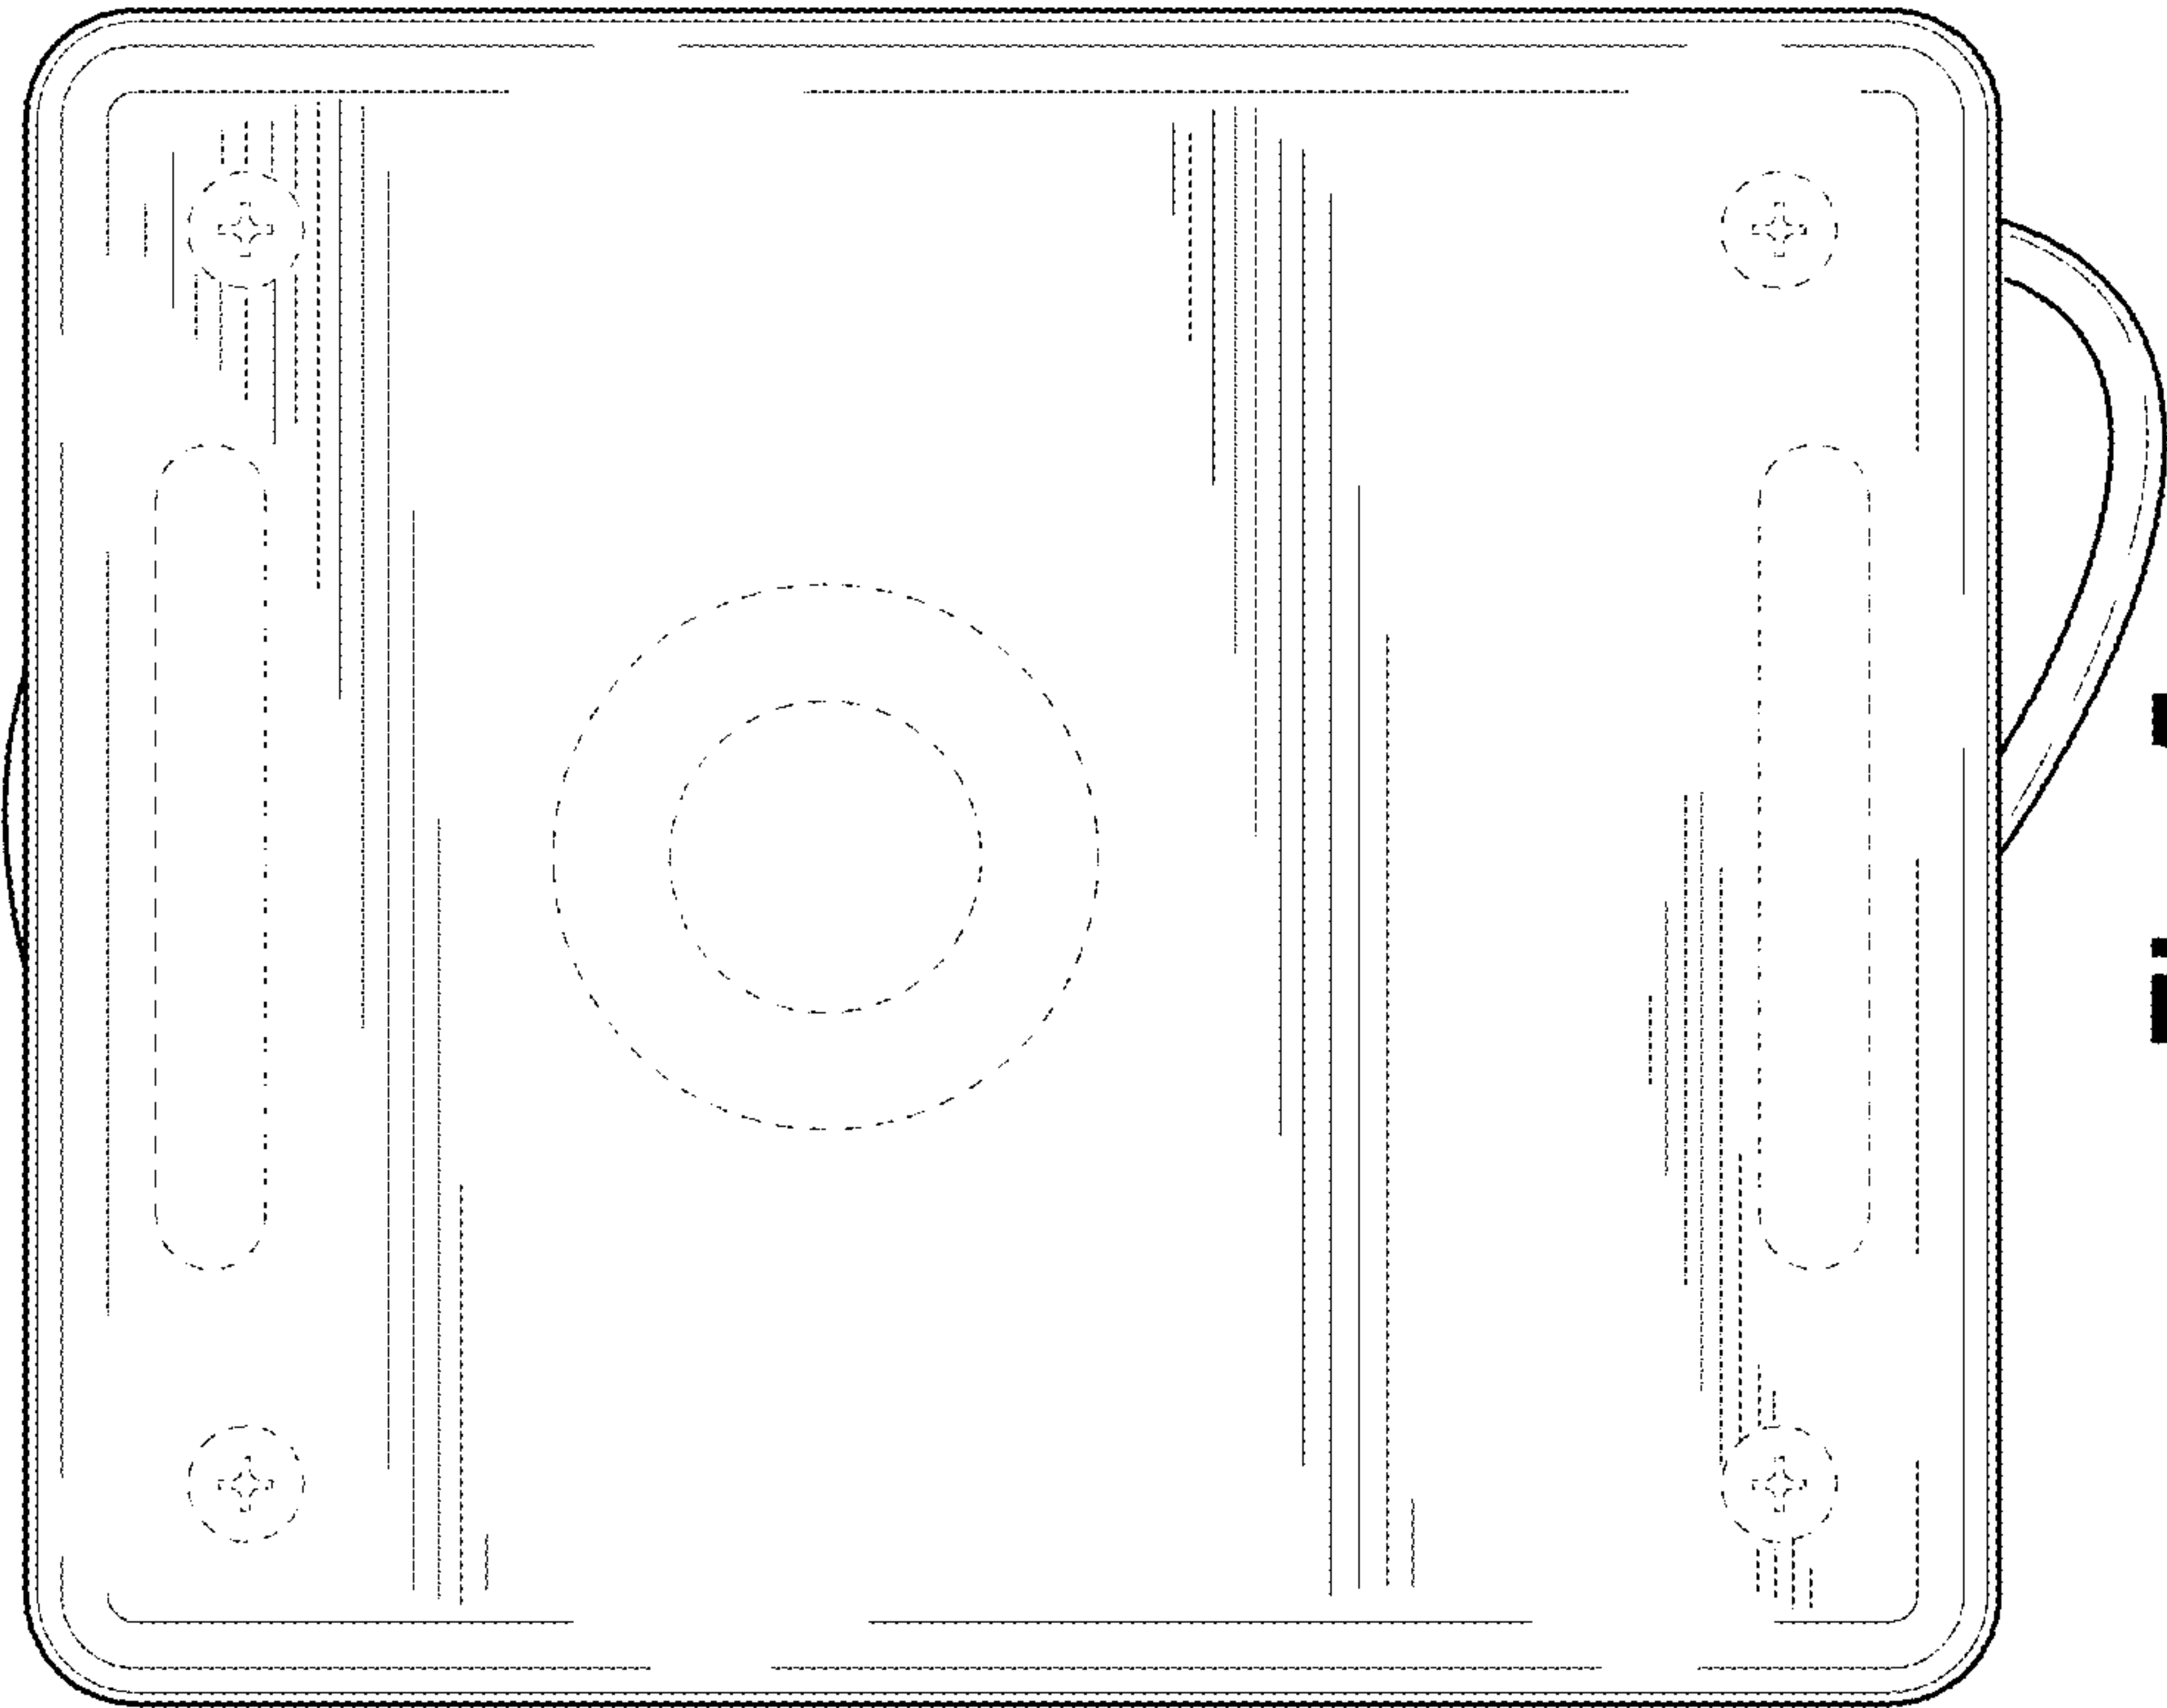


Fig. 5

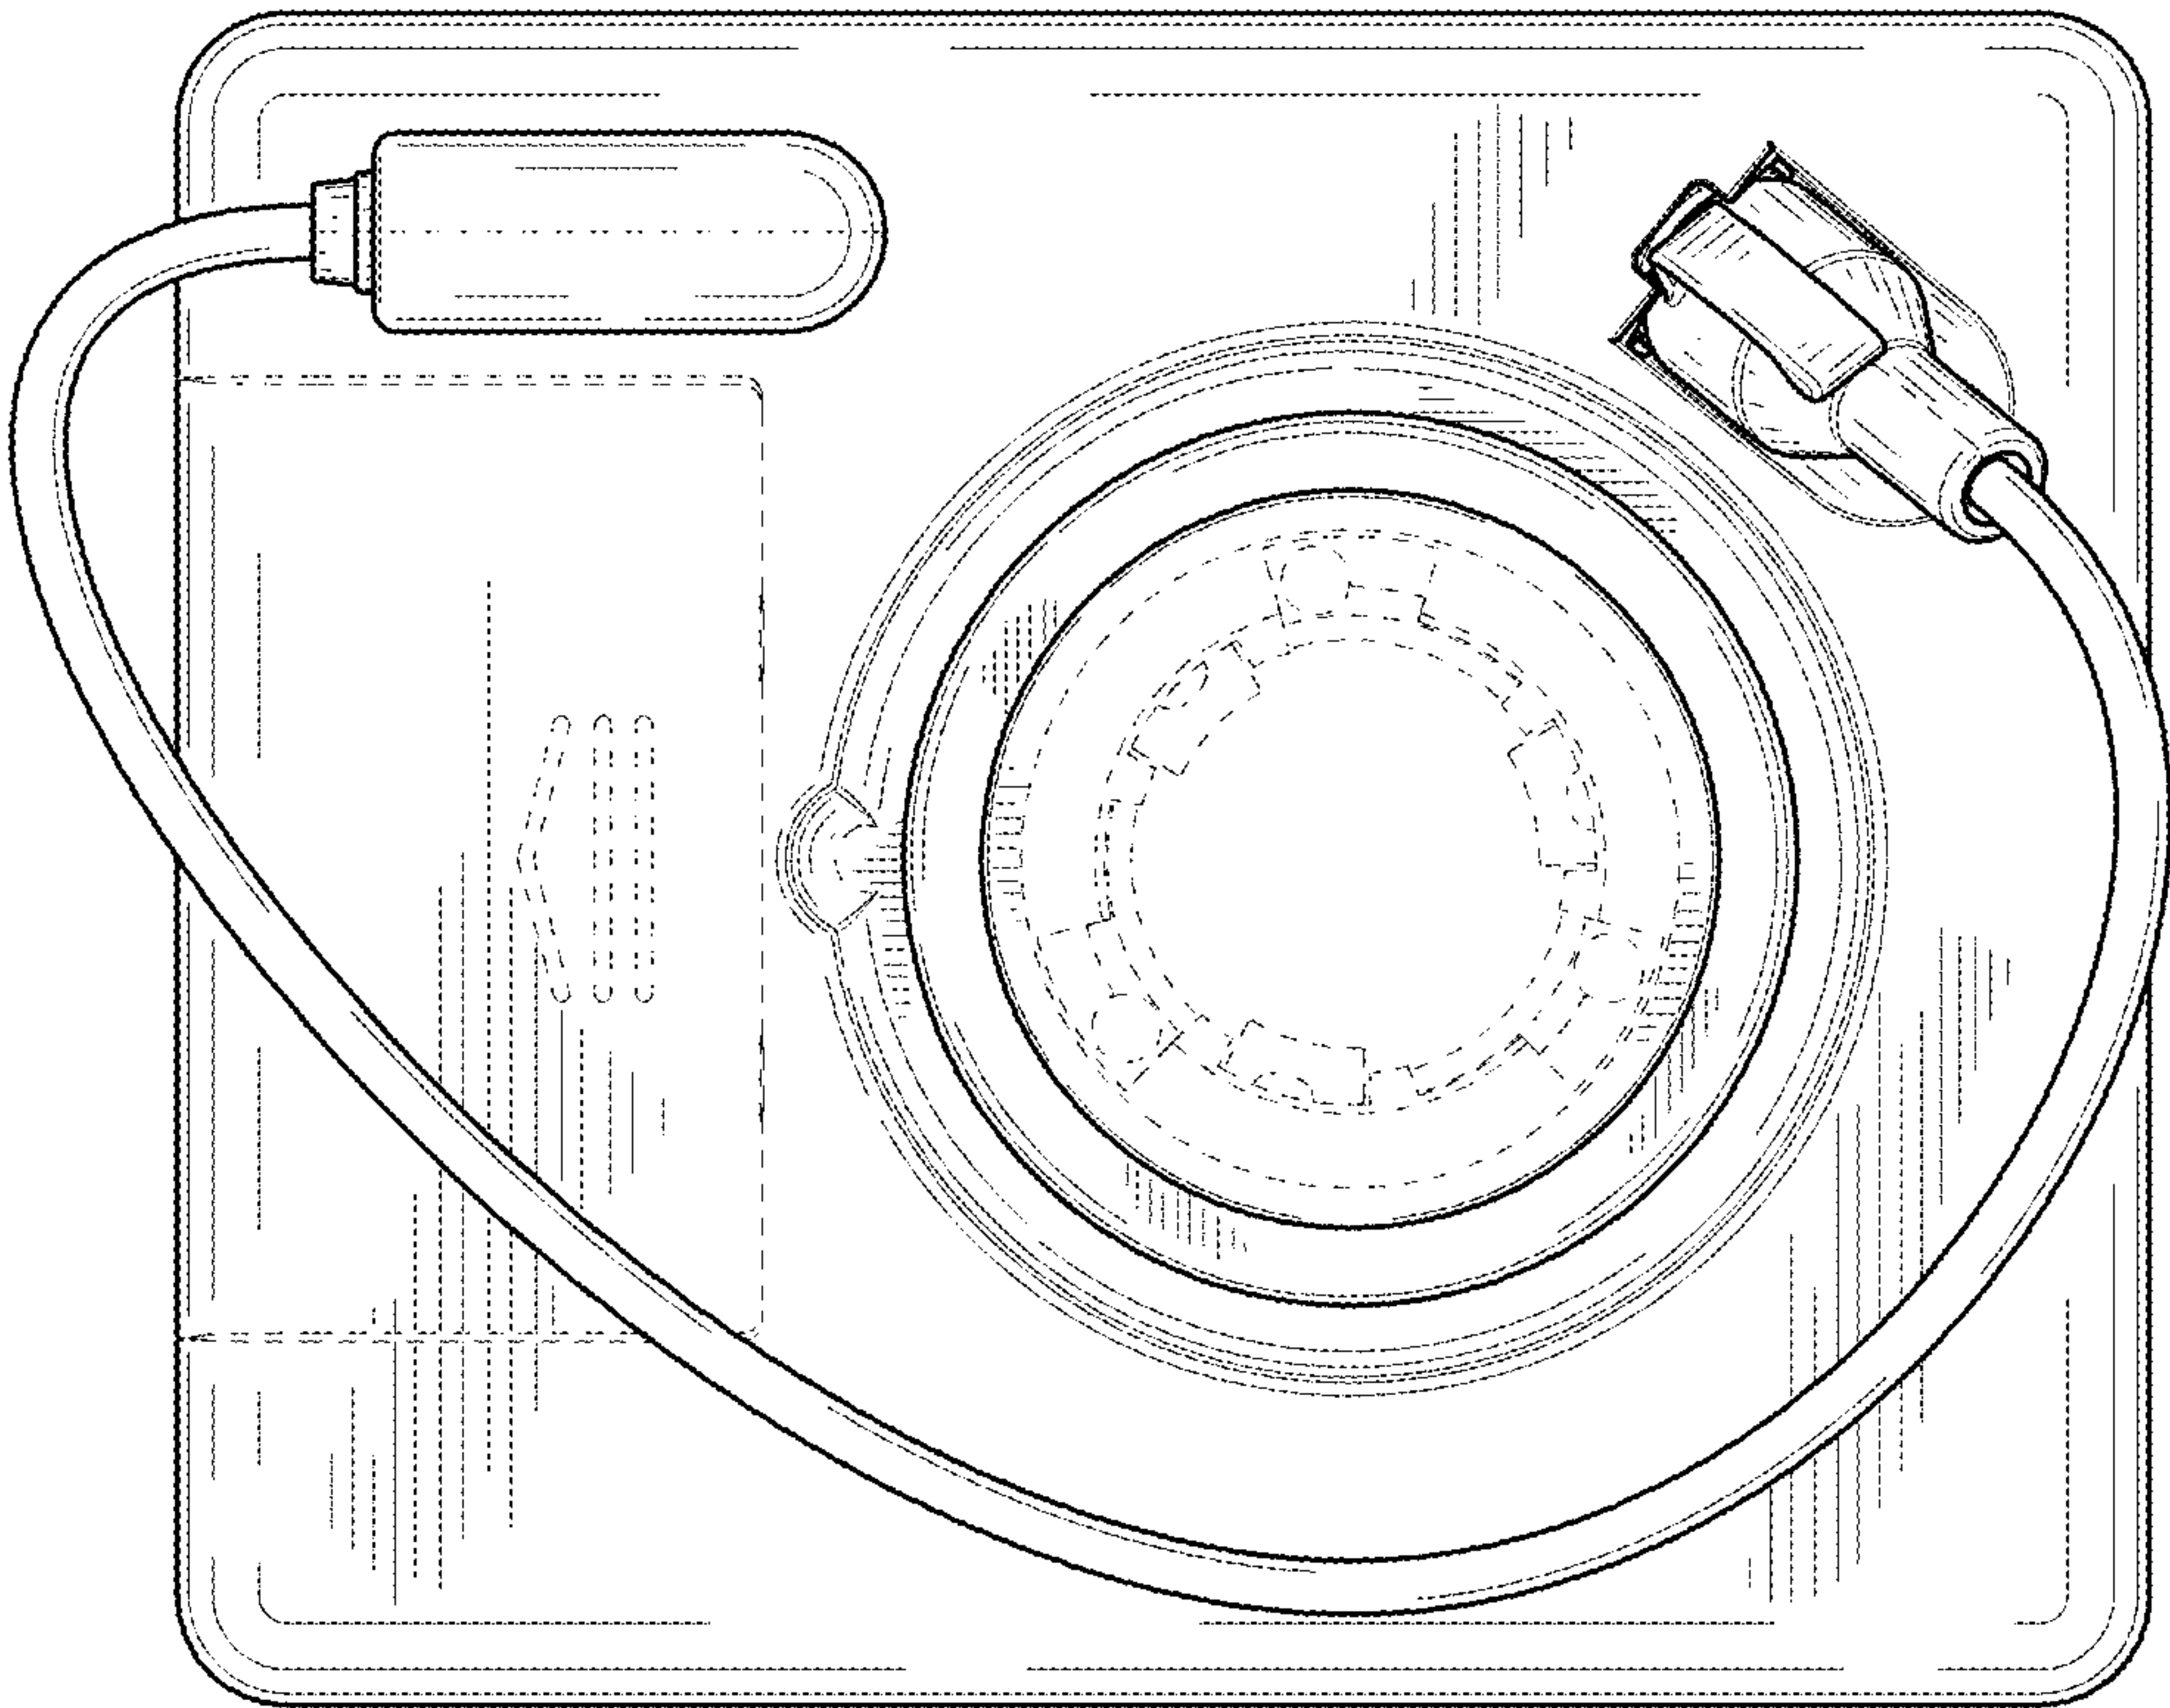


Fig. 4

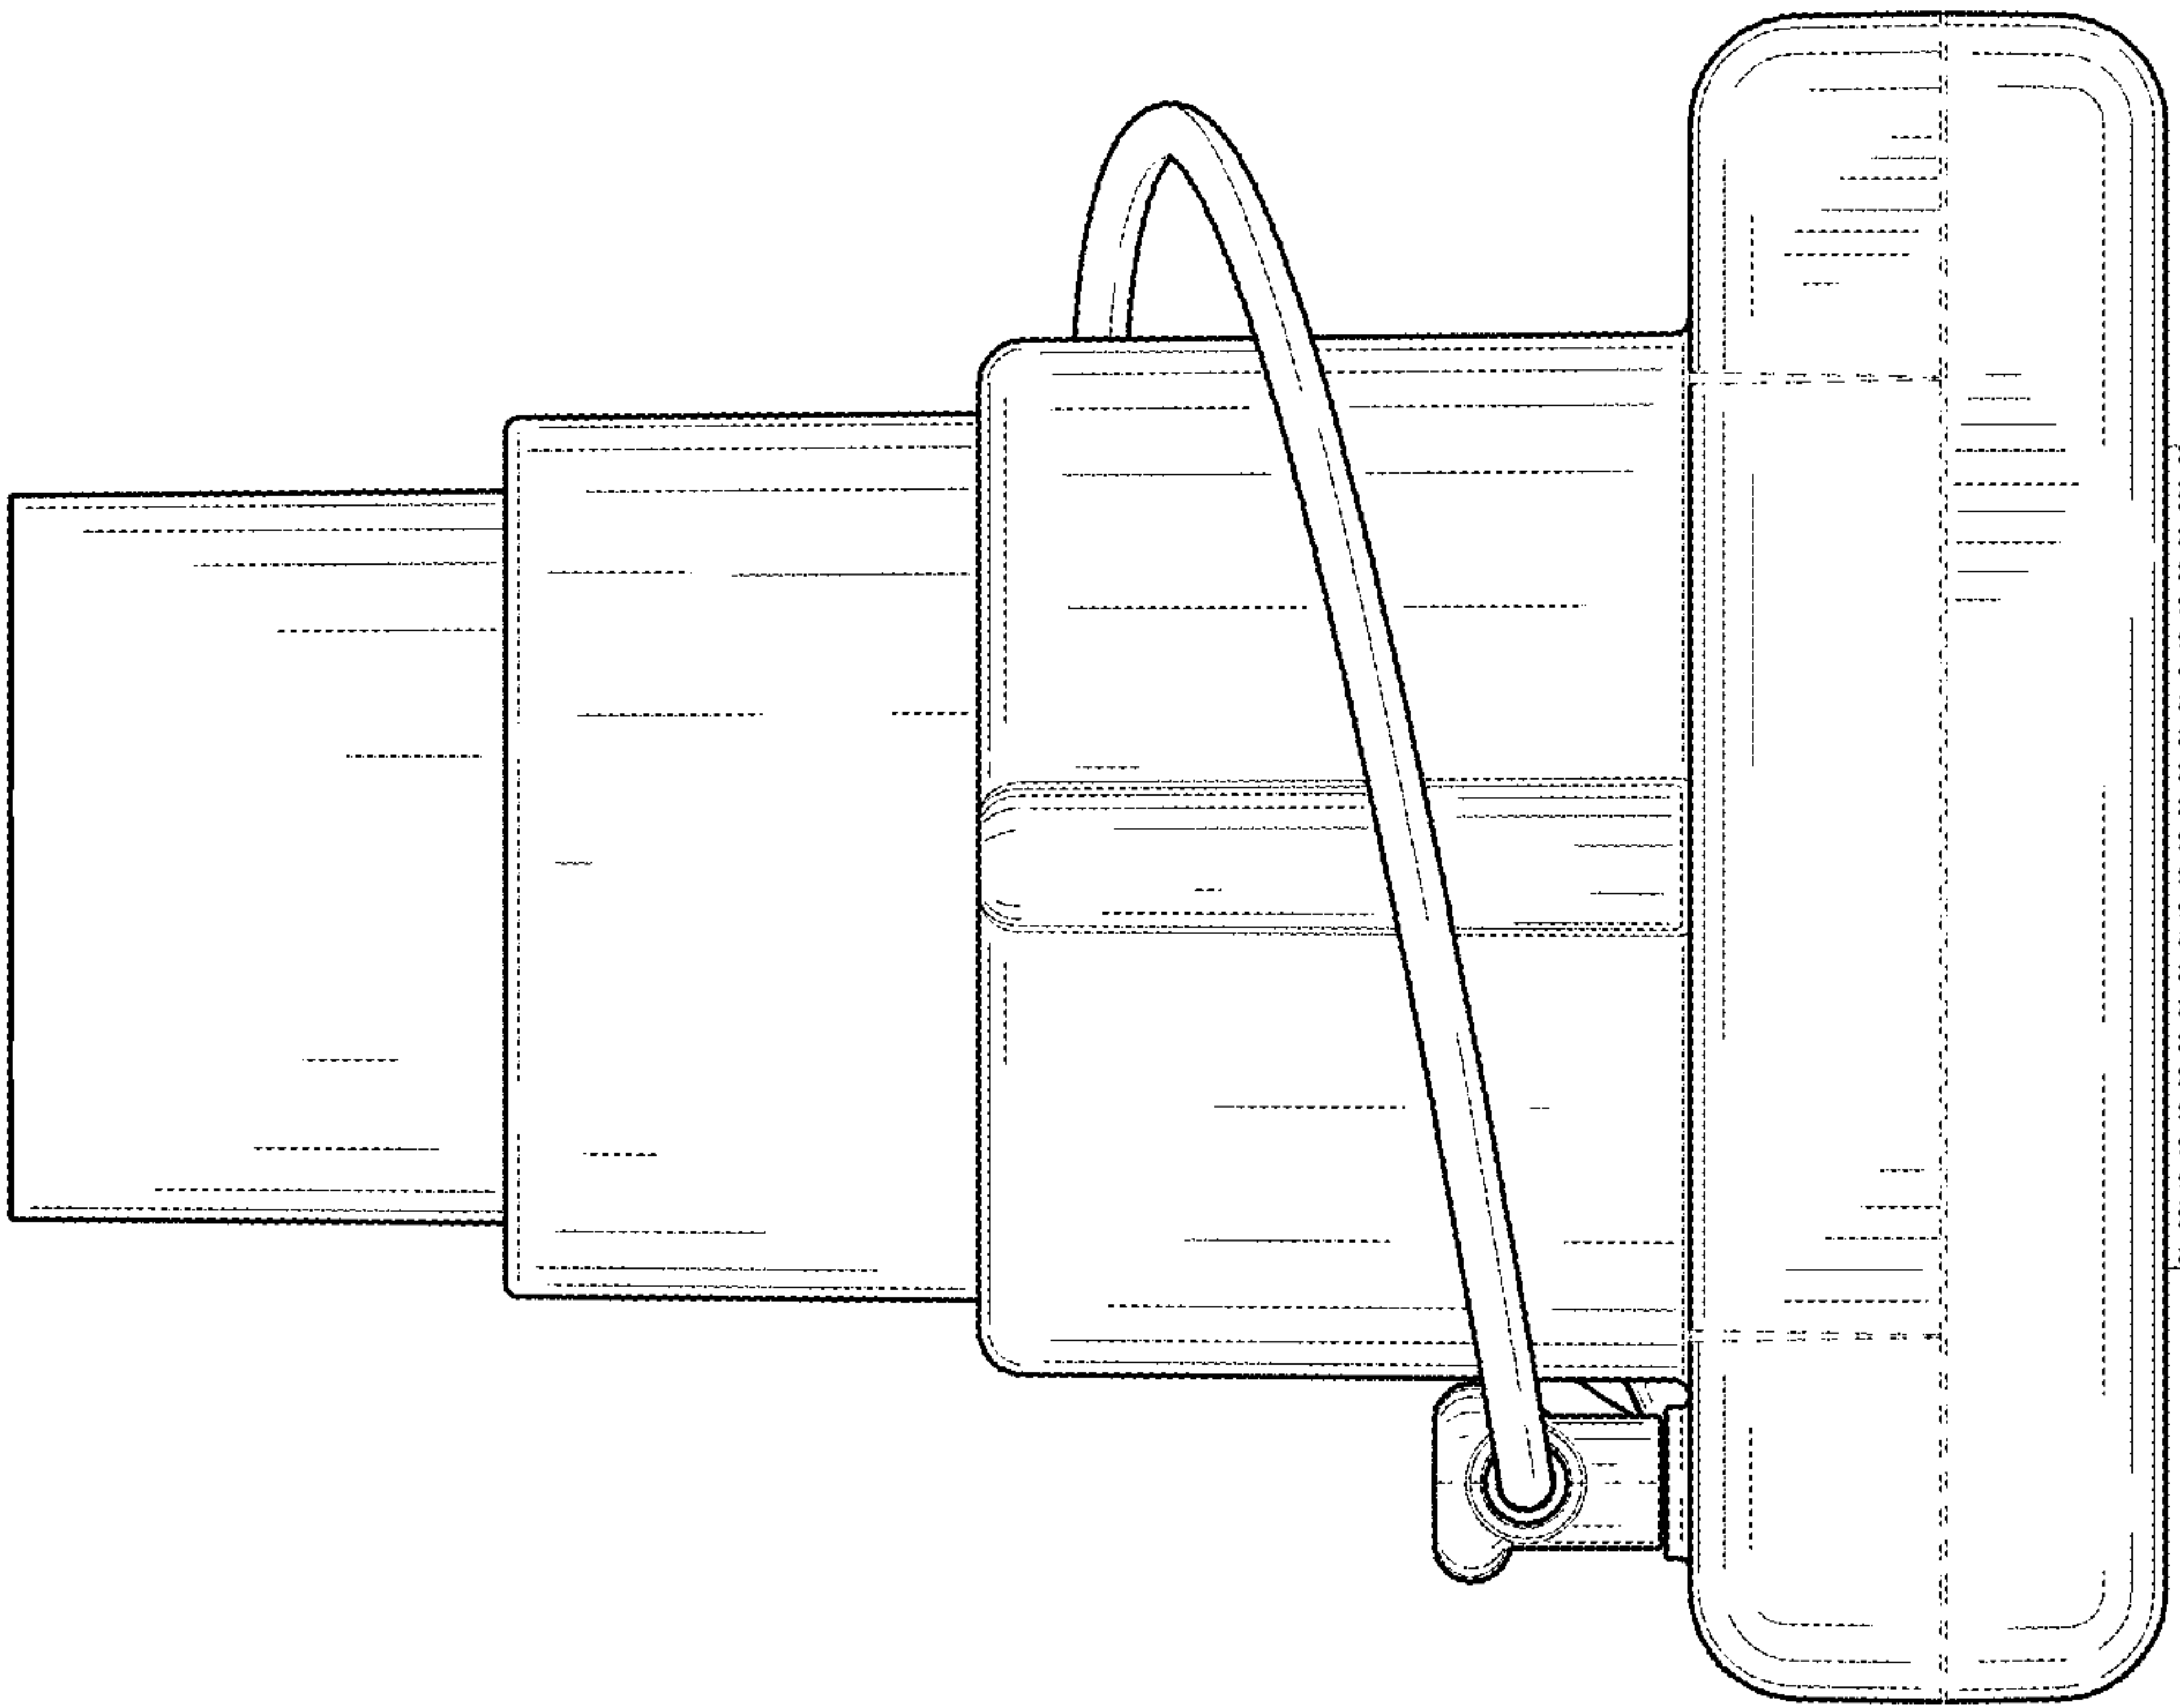


Fig. 7

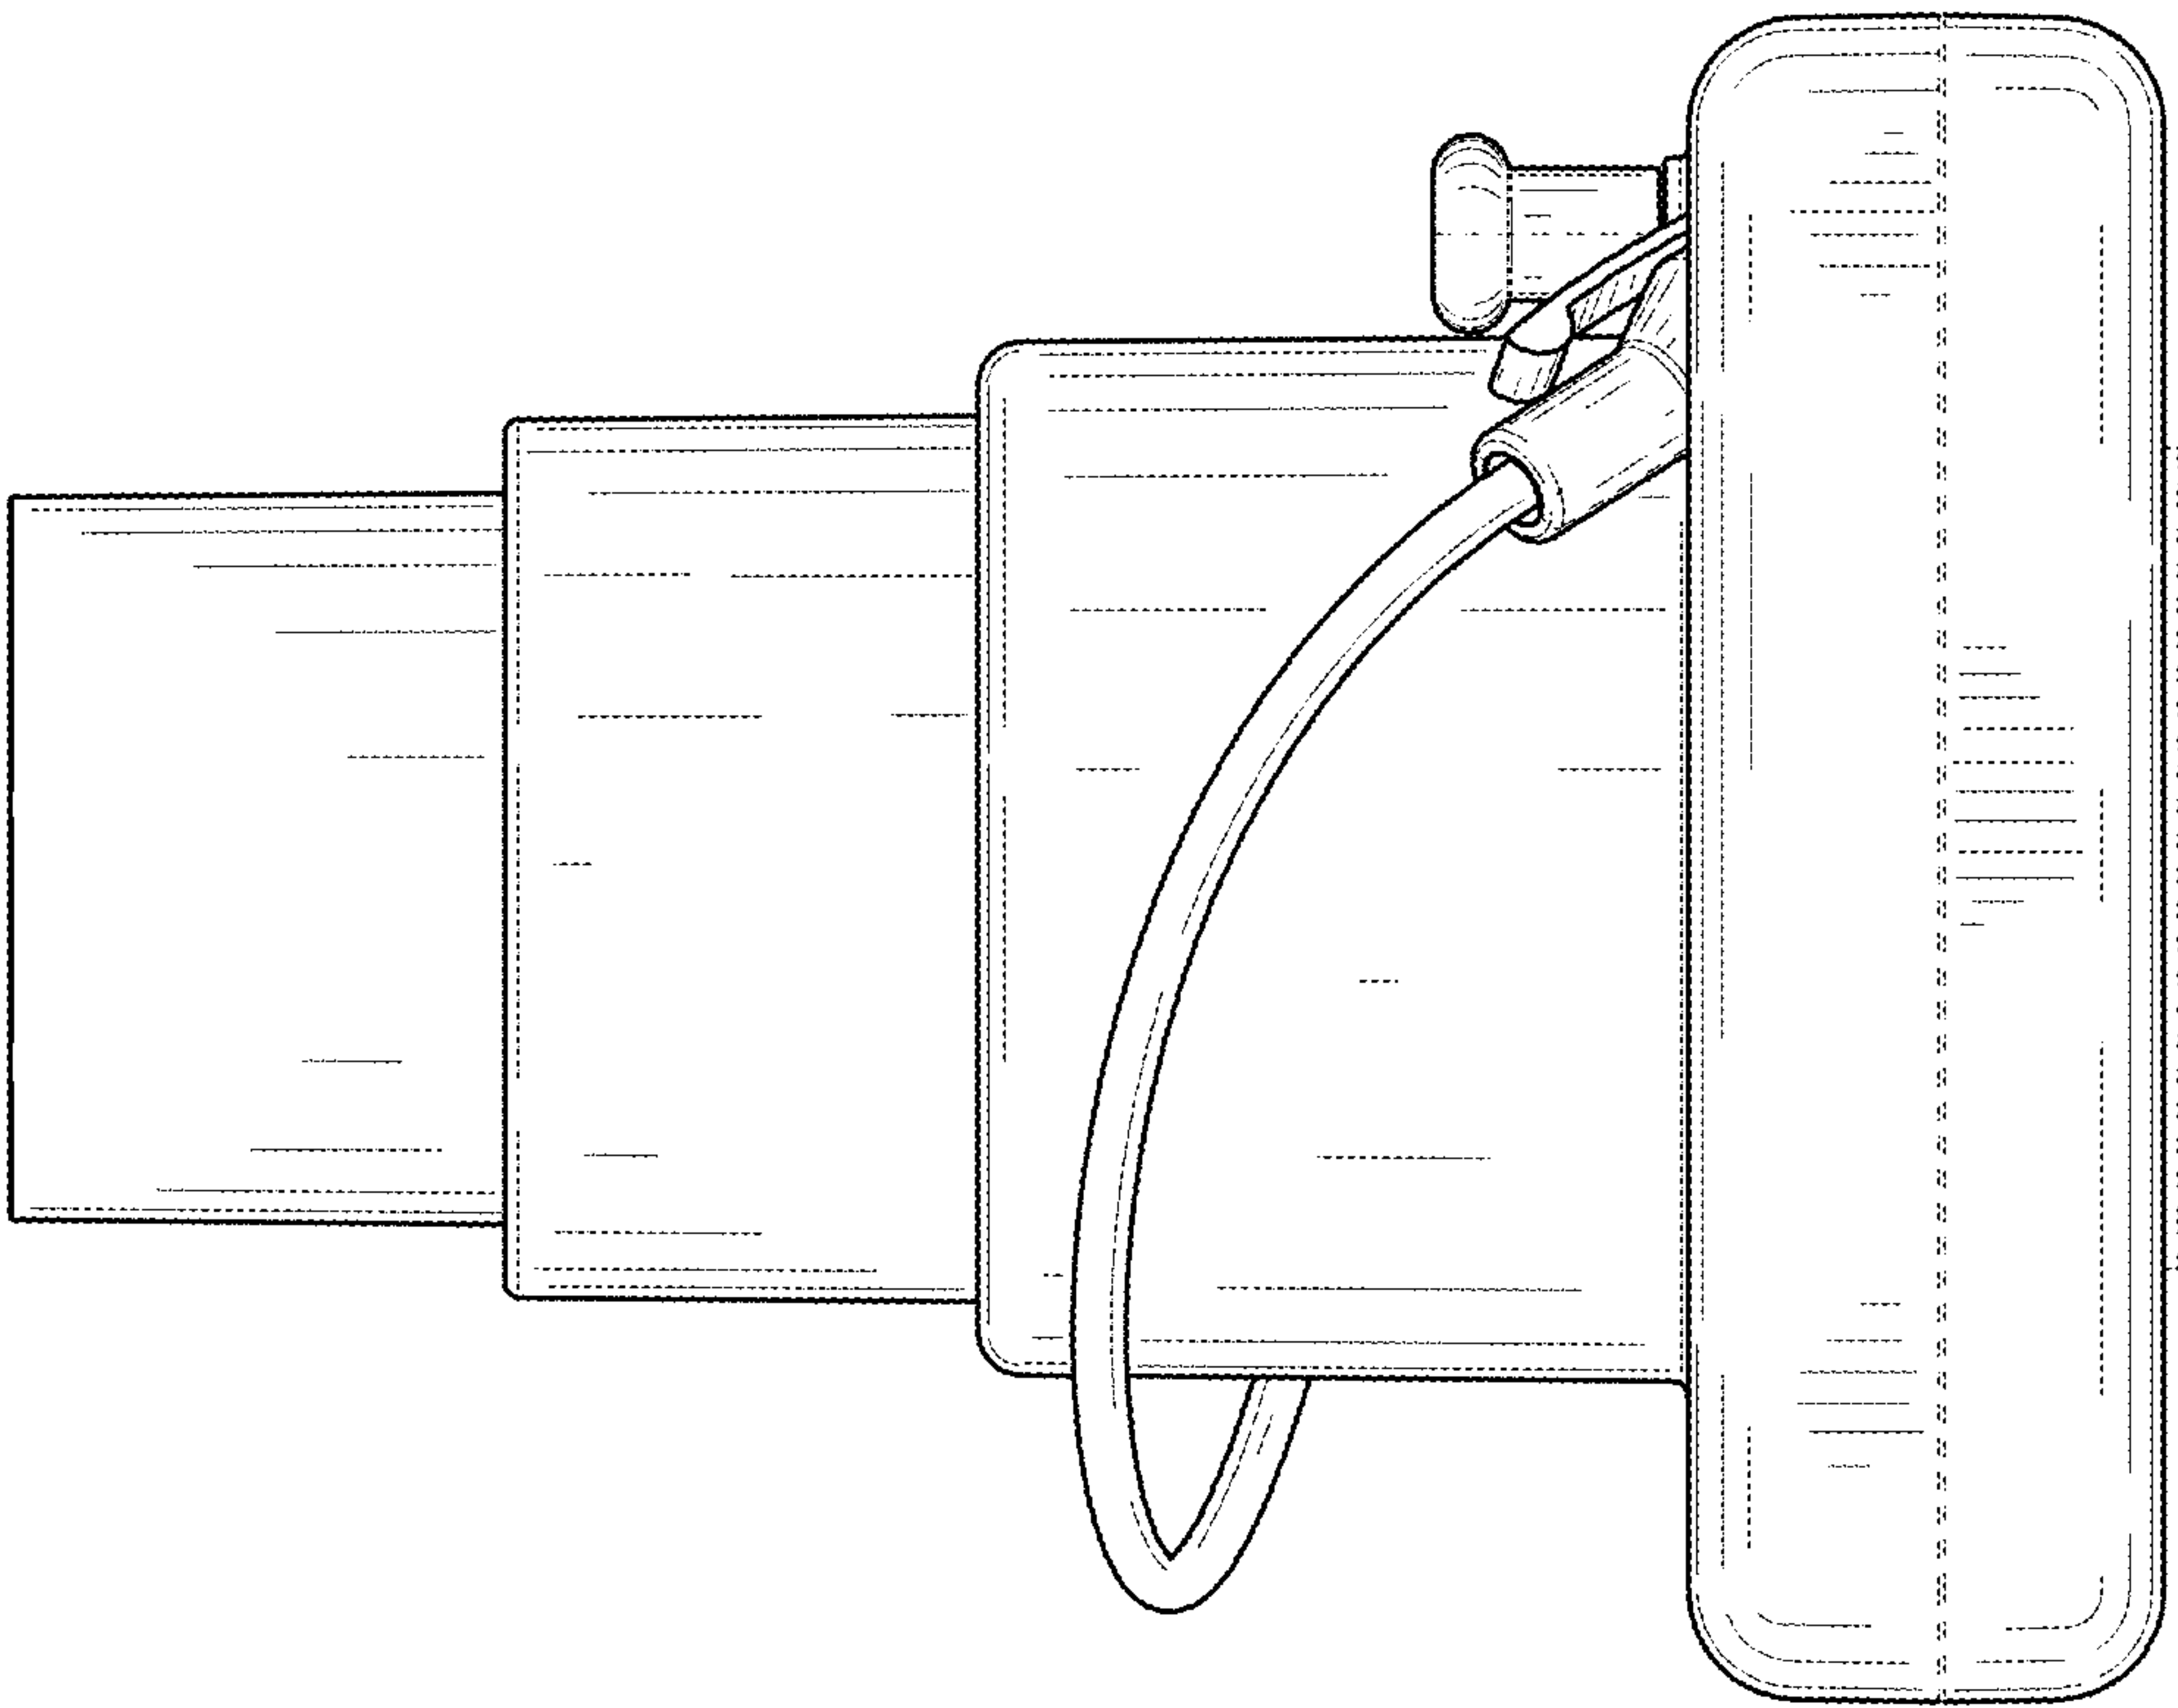


Fig. 6

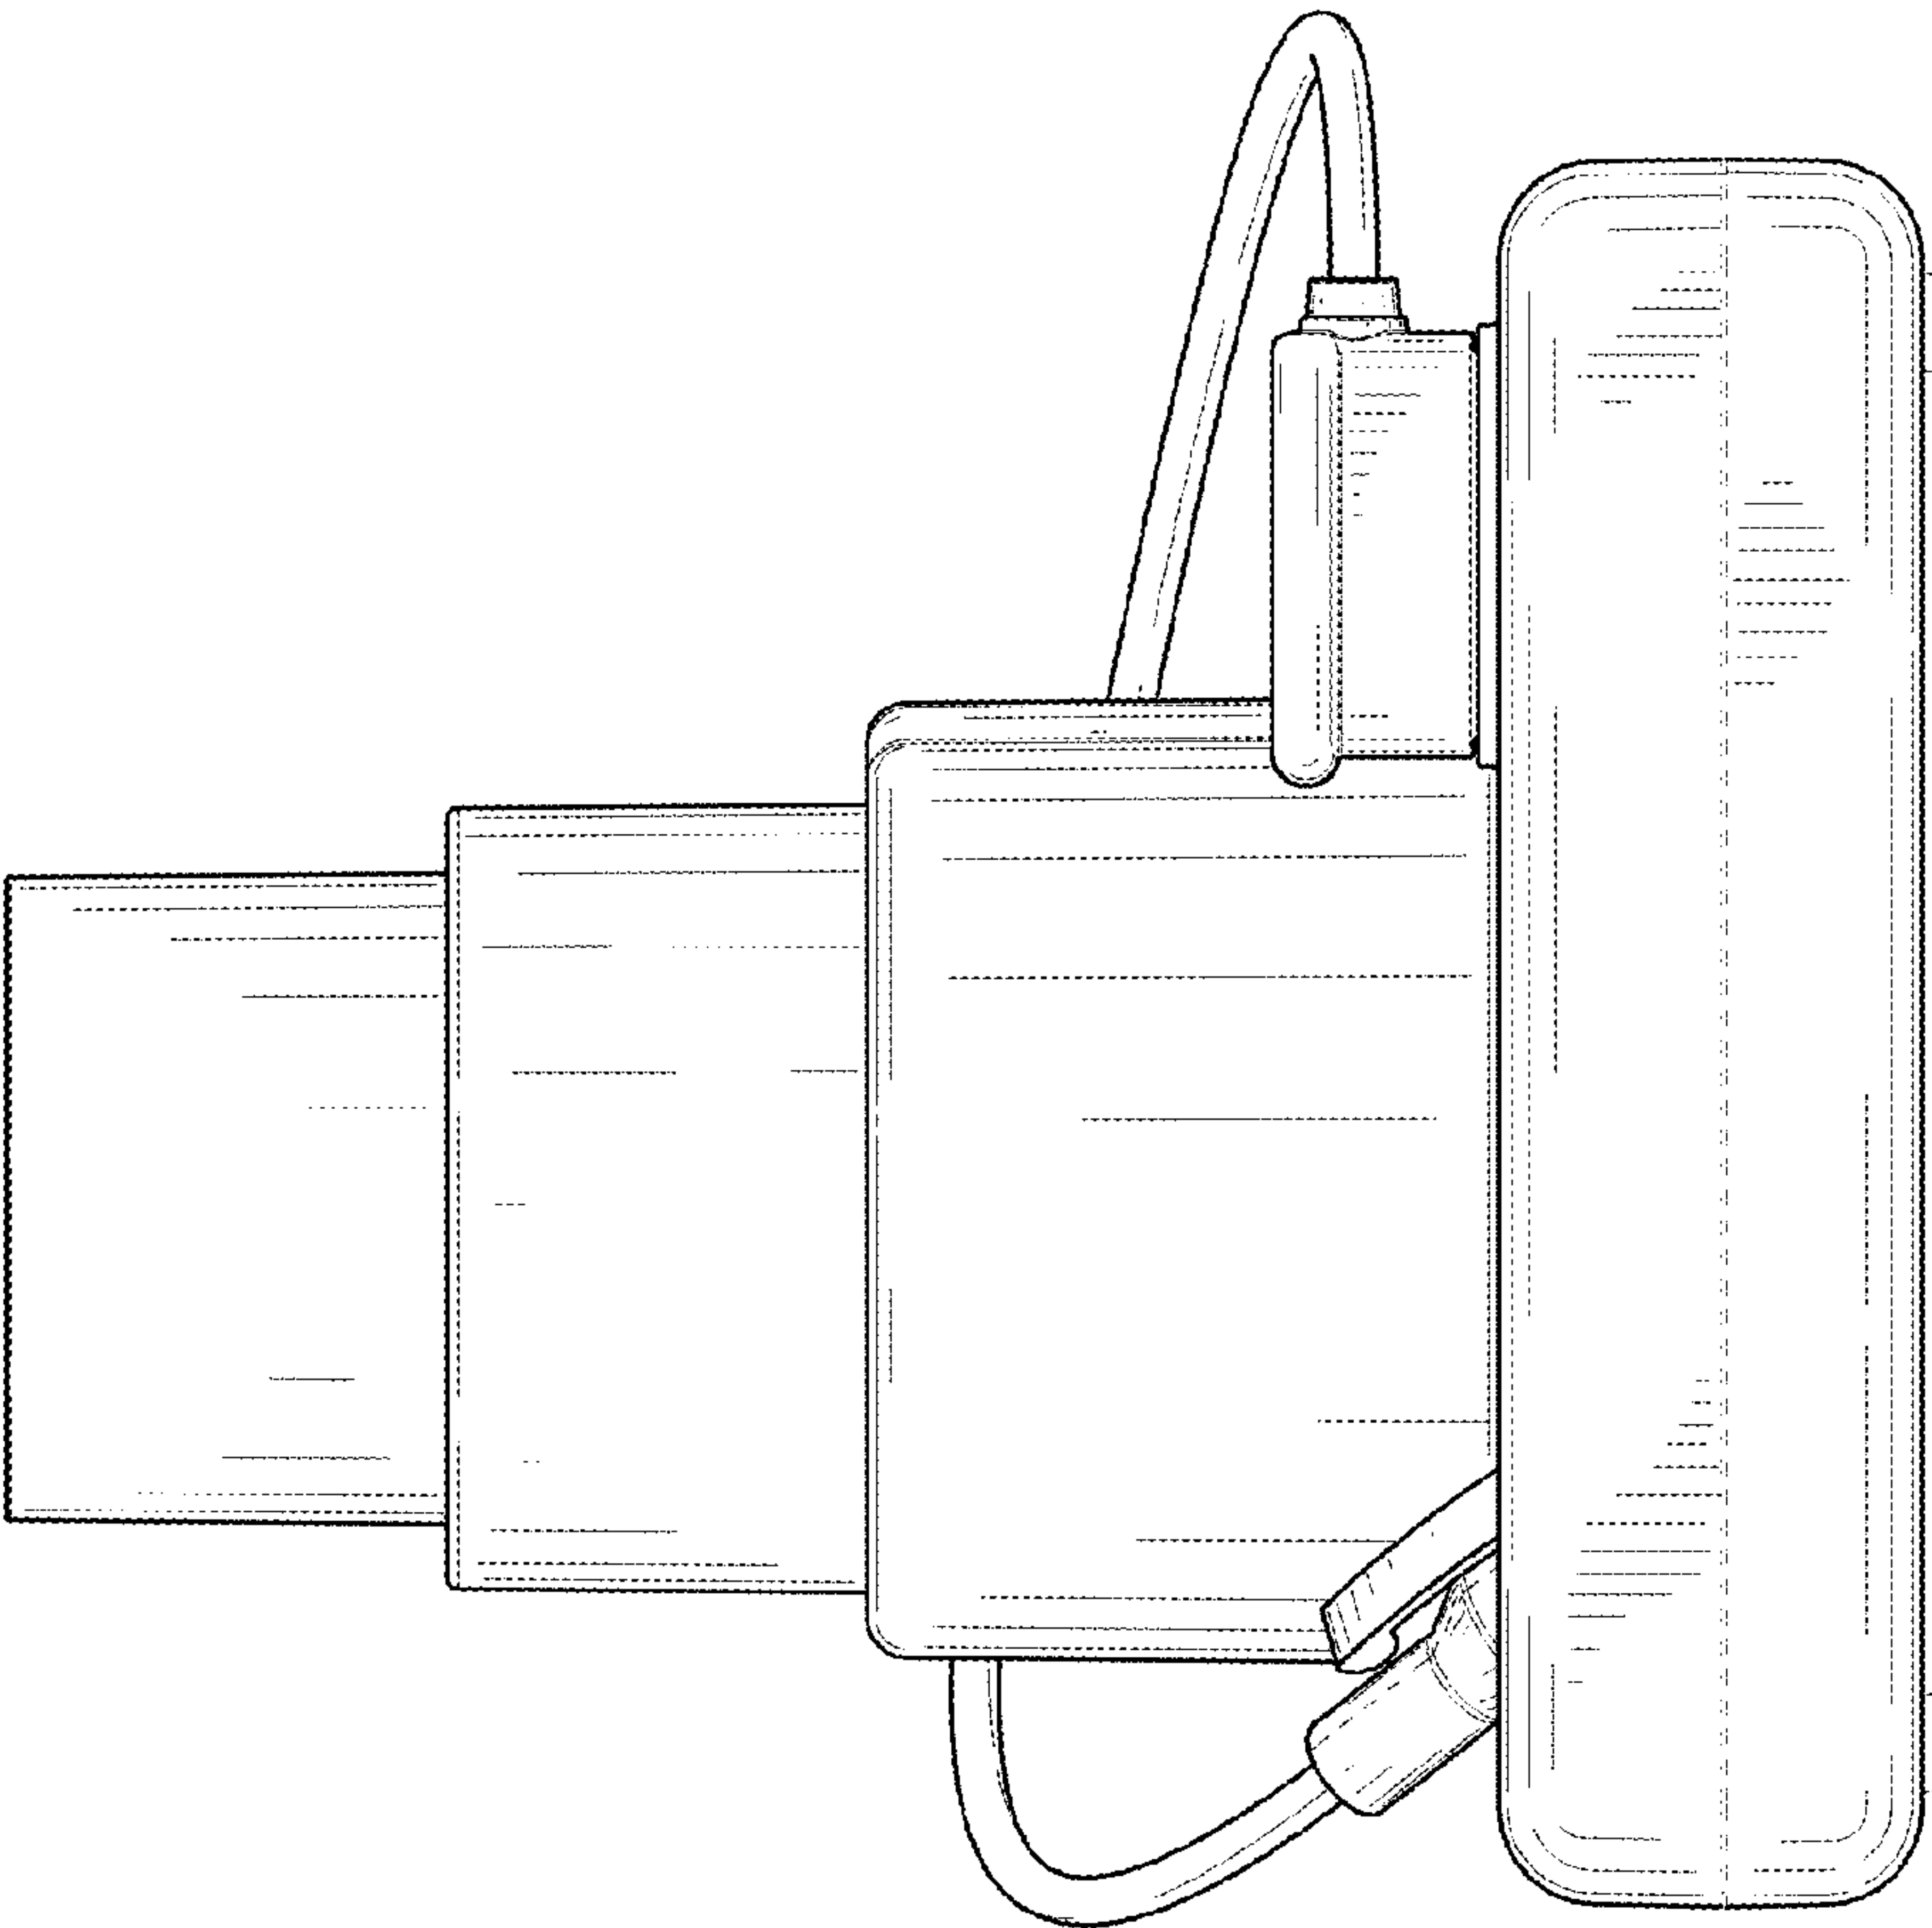


Fig. 9

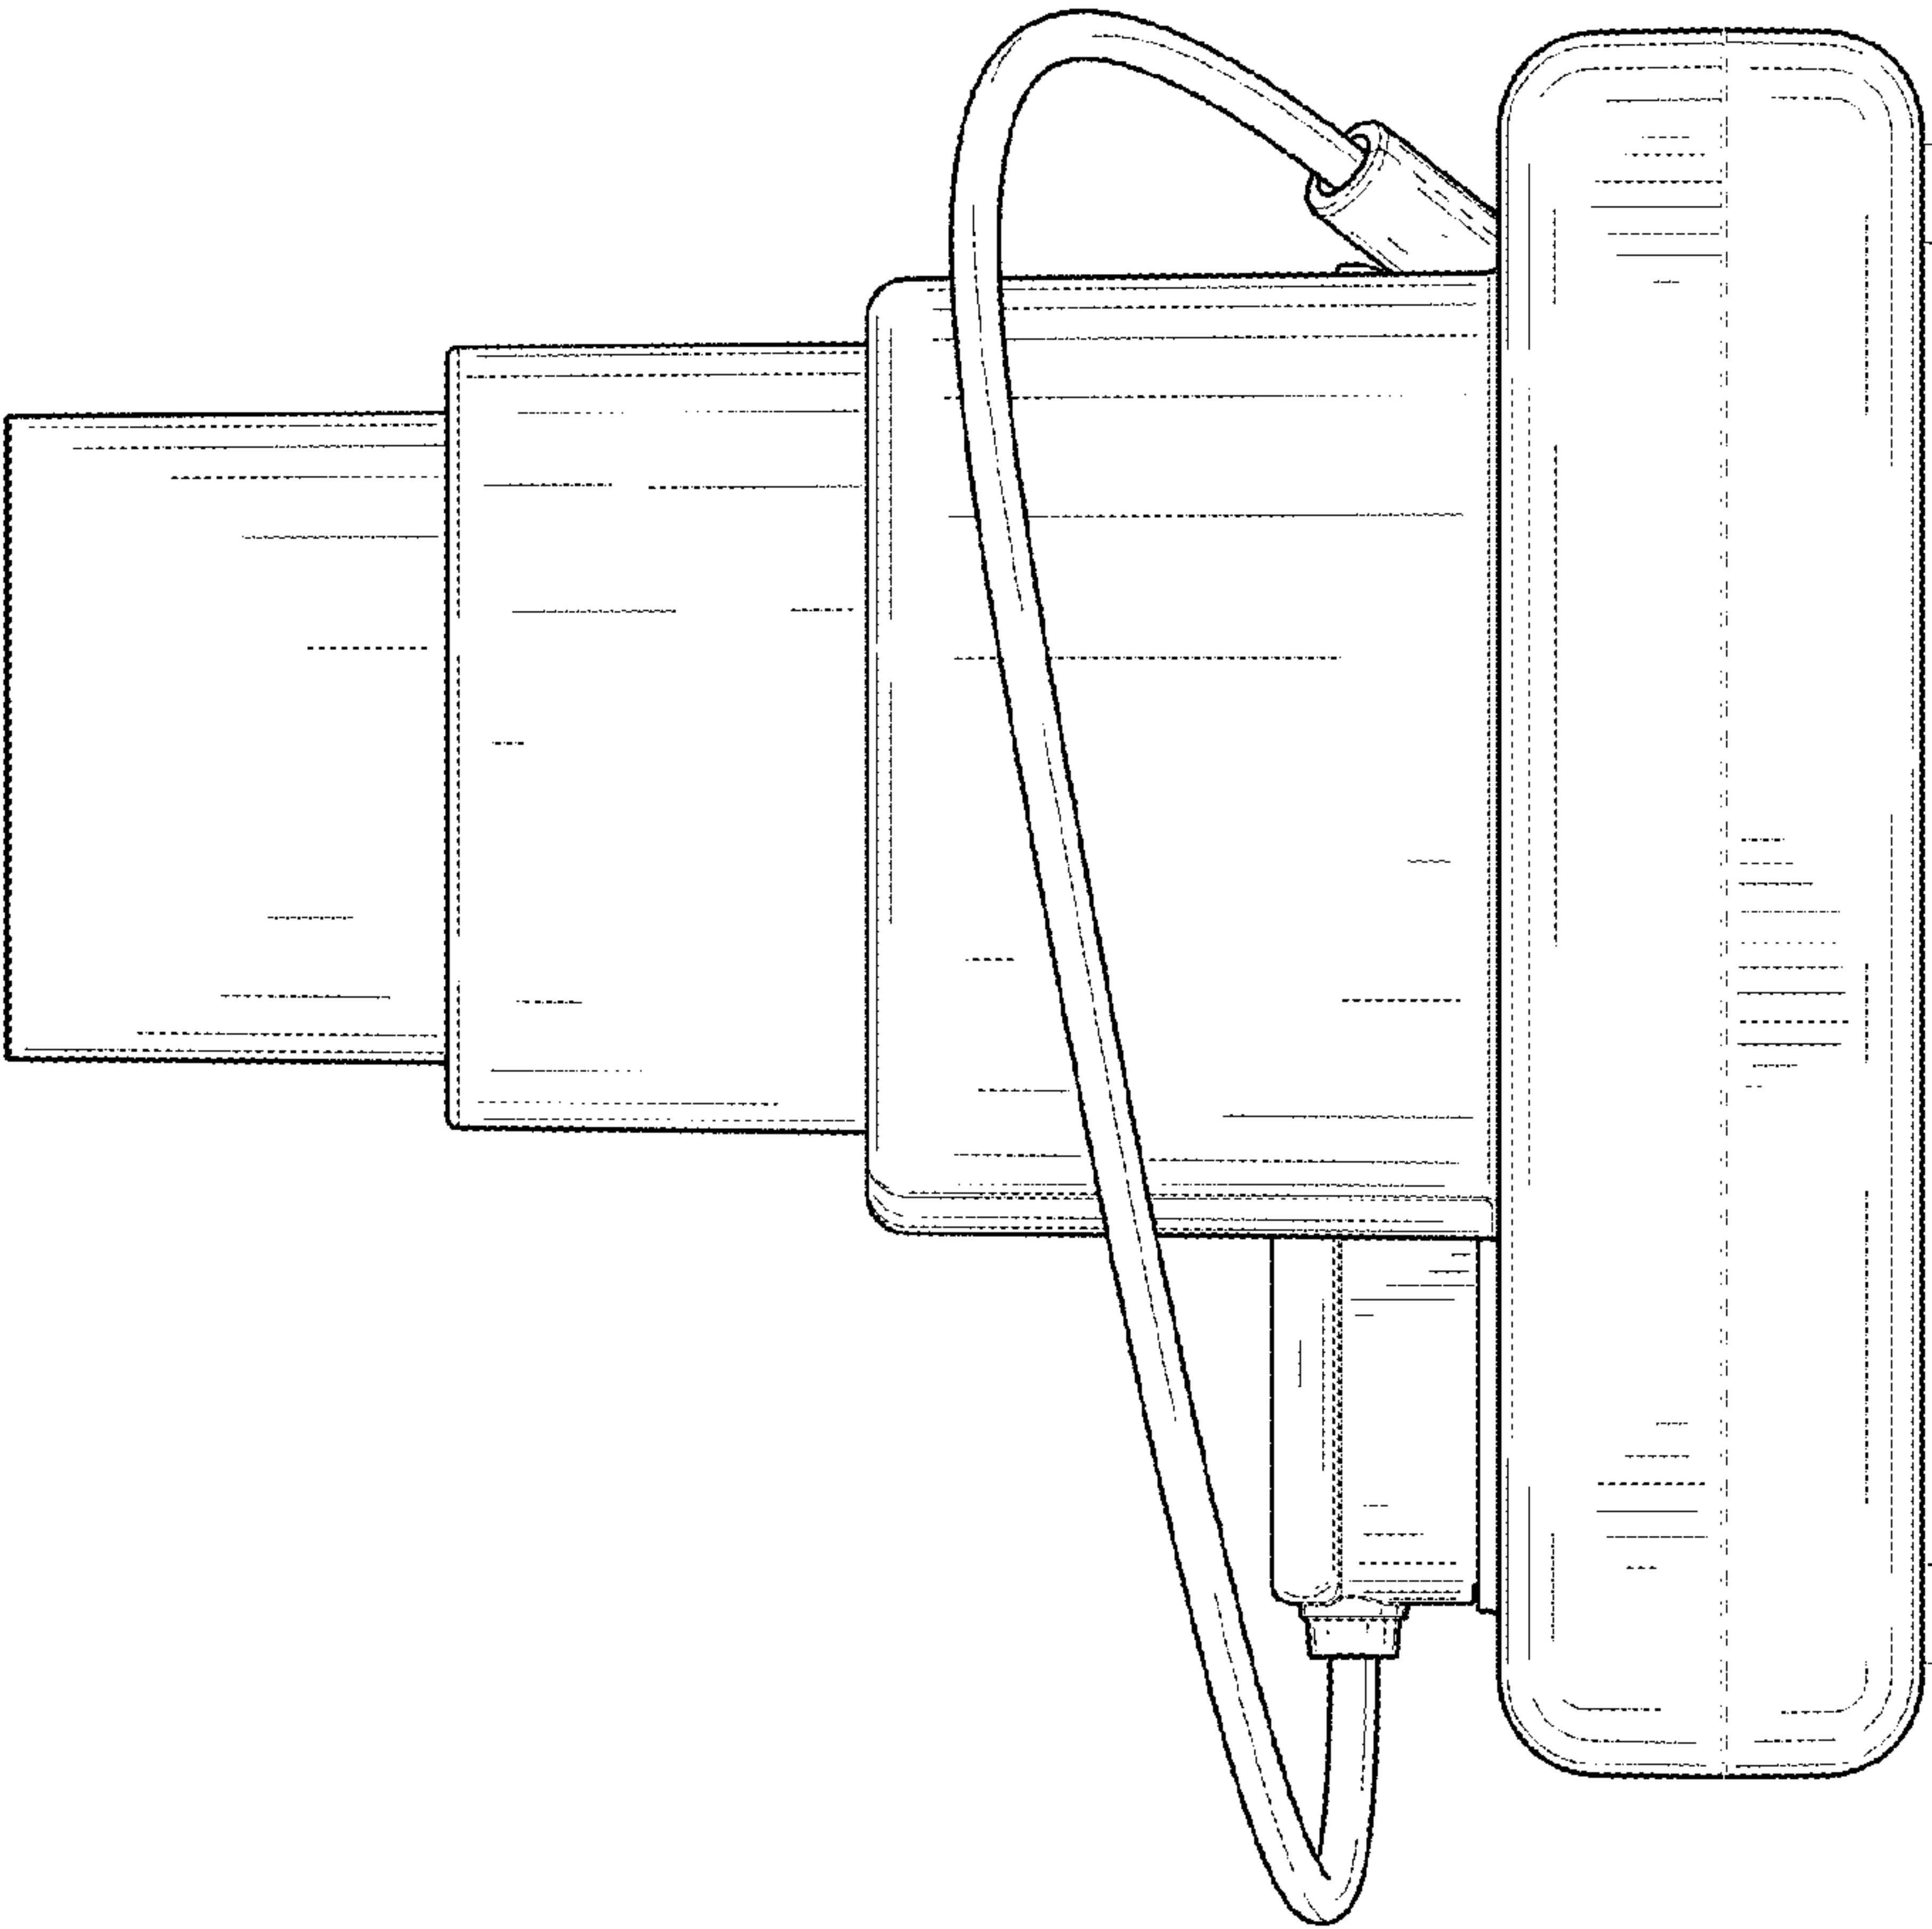


Fig. 8

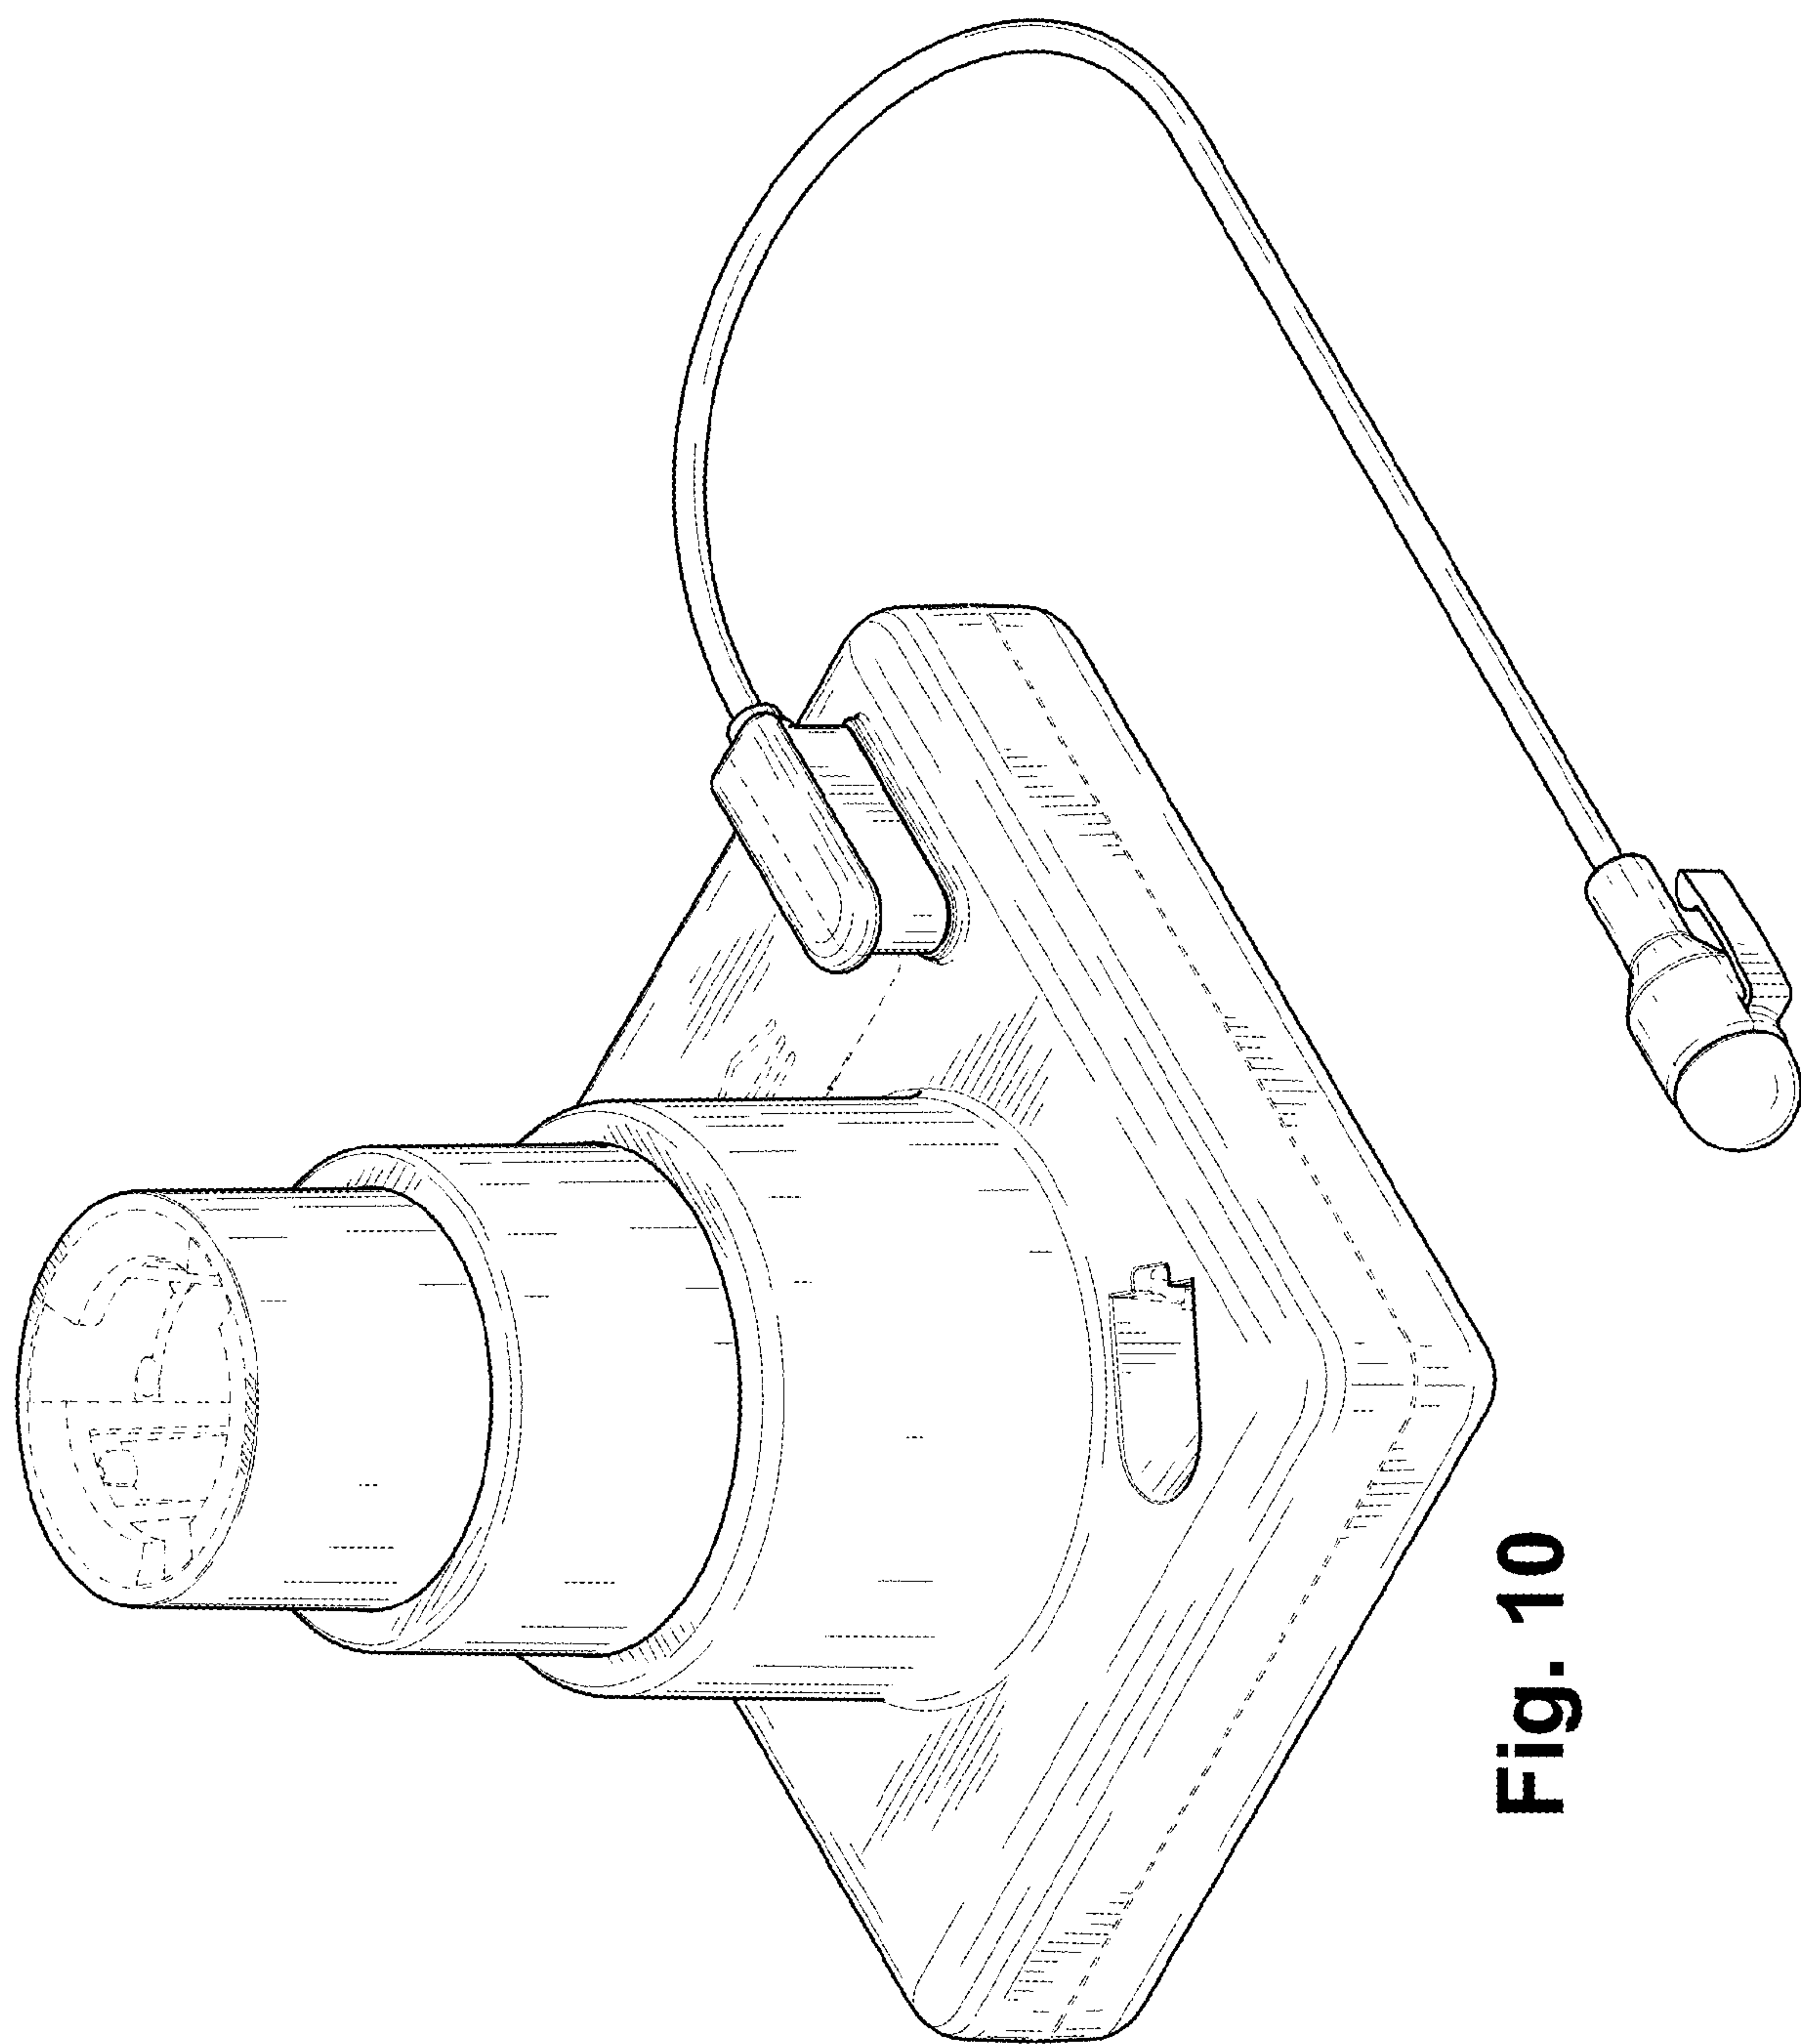


Fig. 10

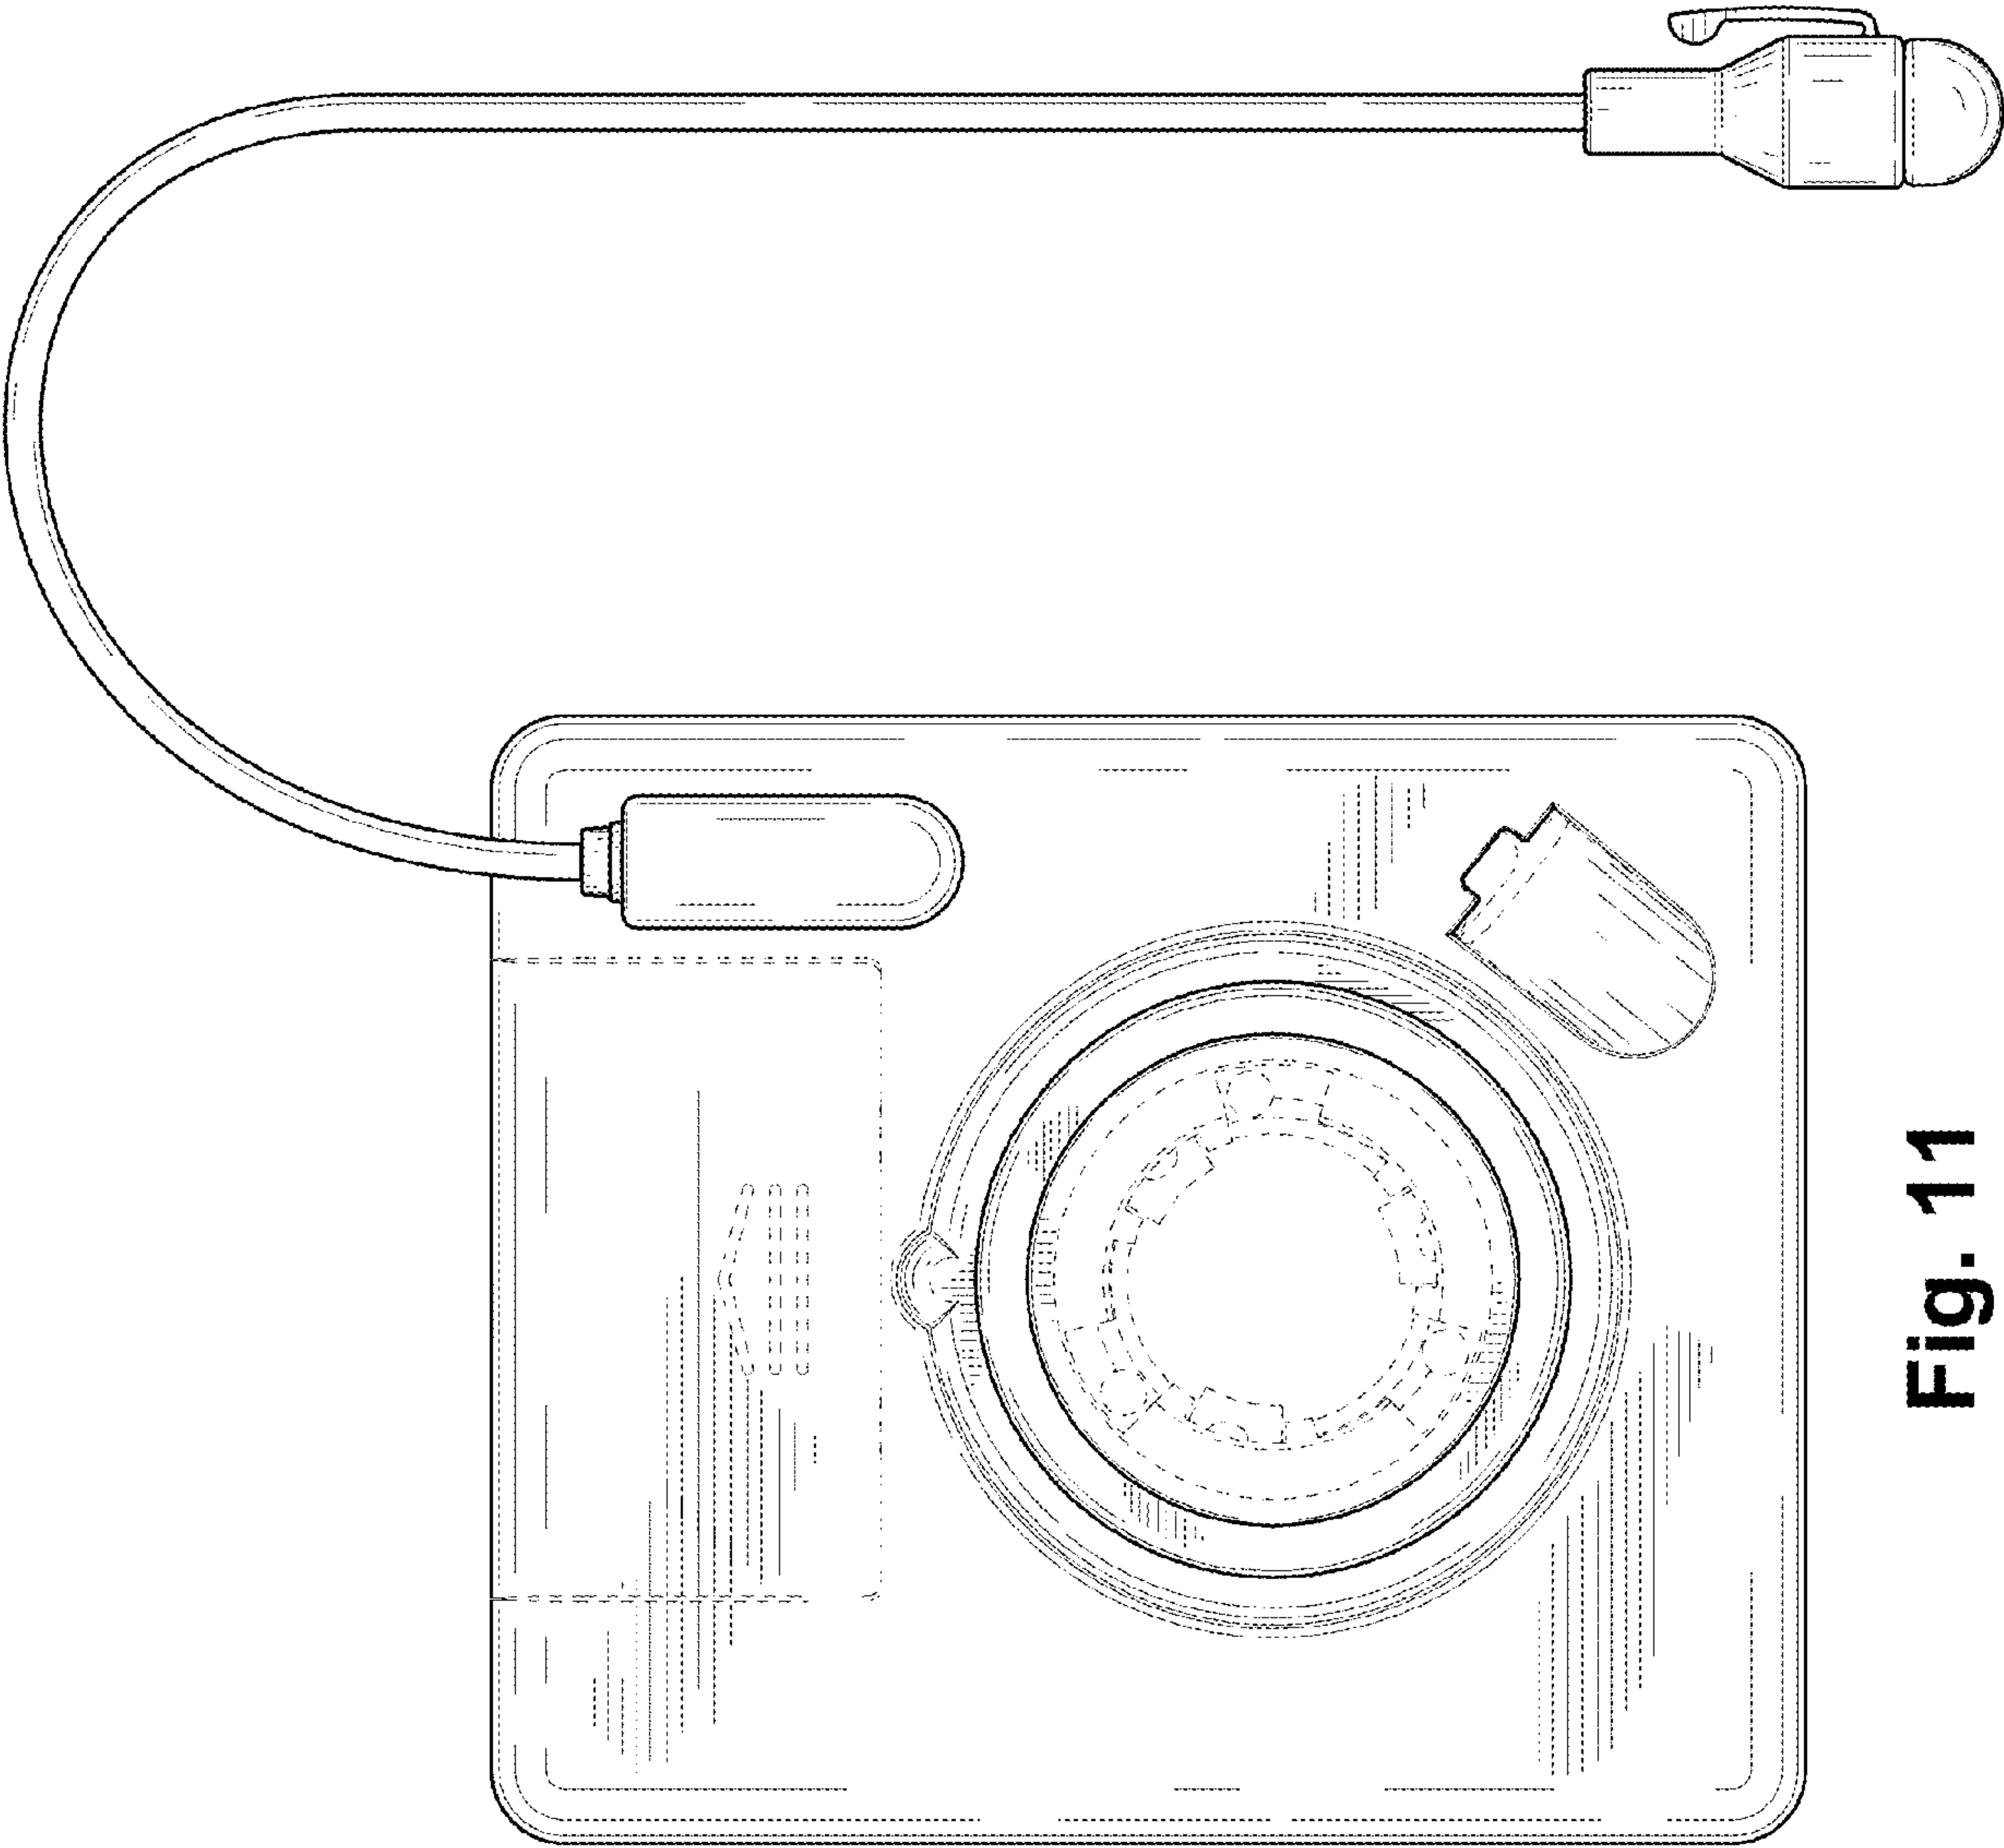


Fig. 11