



US0D1027180S

(12)

United States Design Patent

Roth

(10)

Patent No.:

US D1,027,180 S

(45)

Date of Patent:

** May 14, 2024

(54) MEDICAL IMAGING DEVICE

(71) Applicant: Siemens Healthcare GmbH, Erlangen (DE)

D748,264 S * 1/2016 Dörre D24/158
D796,043 S * 8/2017 Boehner D24/158
D868,260 S * 11/2019 Achleitner D24/158
(Continued)

(72) Inventor: Nadja Roth, Bamberg (DE)

(73) Assignee: Siemens Healthineers AG, Erlangen (DE)

FOREIGN PATENT DOCUMENTS

CN 306581970 * 5/2022
EM 008747828-0001 * 11/2021
EM 008780027-0002 * 12/2021
IN 308891-0001 * 12/2021

(**) Term: 15 Years

OTHER PUBLICATIONS

“Endovascular Today: Siemens Healthineers’ Artis Icono Ceiling Angiography System Cleared by FDA.” Found online at evtoday.com. Oct. 4, 2023. Reference dated Jul. 28, 2022. Retrieved from <https://evtoday.com/news/siemens-healthineers-artis-icono-ceiling-angiography-system-cleared-by-fda-1>.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton
Assistant Examiner — Elizabeth S Struble
(74) Attorney, Agent, or Firm — Banner & Witcoff Ltd.

(30) Foreign Application Priority Data

Nov. 29, 2021 (EM) 008780027-0001
Nov. 29, 2021 (EM) 008780027-0002
Nov. 29, 2021 (EM) 008780027-0003

(51) LOC (14) Cl. 24-01

(52) U.S. Cl.
USPC D24/158

(58) Field of Classification Search
USPC D24/107, 158, 159, 160, 161, 183, 184,
D24/185, 186, 216, 232
CPC .. A61B 5/05; A61B 5/055; A61B 6/03; A61B
6/035; A61B 6/4411; A61B 6/4447; A61B
6/4405; A61B 6/4435; A61B 6/4441;
A61B 8/4405; A61B 8/4411; A61B
8/4427; A61B 8/462; A61B 8/0437;
G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
G01N 21/76; G01N 21/6428
See application file for complete search history.

(57) CLAIM

The ornamental design for a medical imaging device, as shown and described.

DESCRIPTION


FIG. 1 is a front view of a medical imaging device showing our new design;
FIG. 2 is a back elevational view thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a bottom plan view thereof;
FIG. 5 is a left-side elevational view thereof;
FIG. 6 is a right-side elevational view thereof; and,
FIG. 7 is a bottom, front, right-hand side perspective view thereof.
The broken lines in the drawings depict portions of the medical imaging device that form no part of the claimed design.

(56) References Cited

U.S. PATENT DOCUMENTS

D658,762 S * 5/2012 Yokoyama D24/158
D673,273 S * 12/2012 Wahlstrom D24/158
D702,837 S * 4/2014 Dinse D24/158

1 Claim, 7 Drawing Sheets

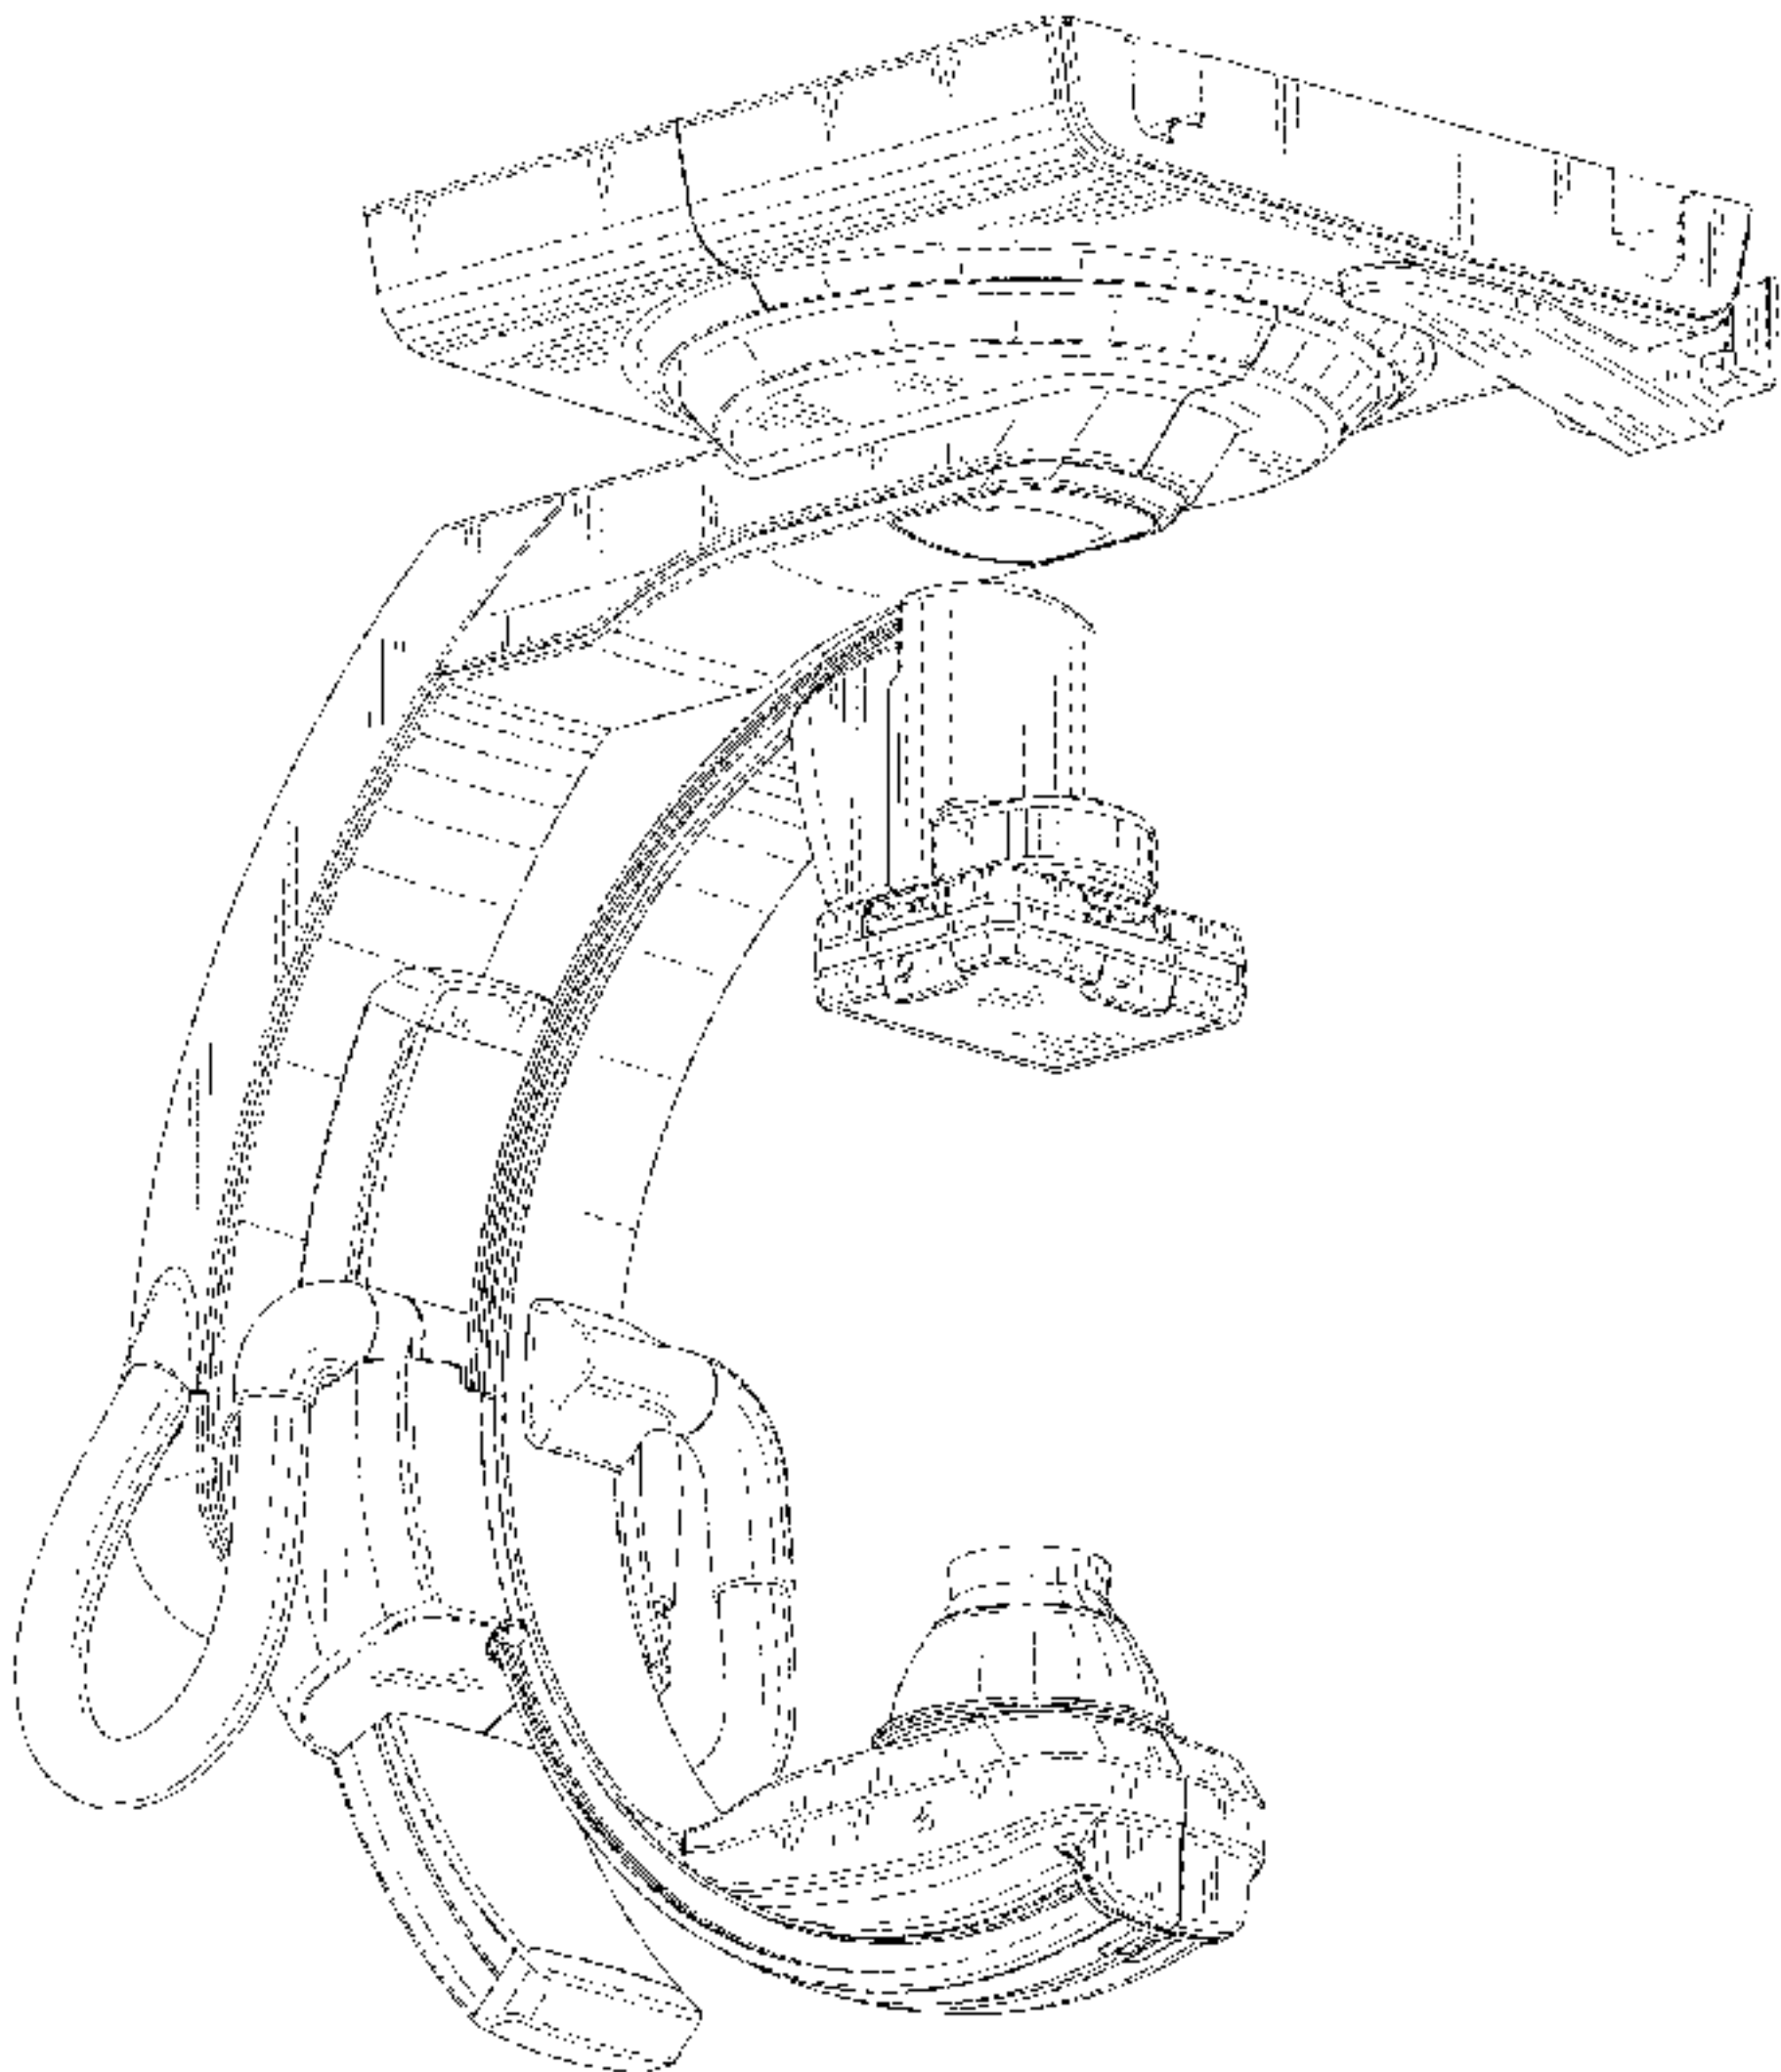

(56) **References Cited**

U.S. PATENT DOCUMENTS

D884,182	S	*	5/2020	Hörndler		D24/158
D895,802	S	*	9/2020	Roth		D24/158
D919,090	S	*	5/2021	Li		D24/158
2018/0132814	A1	*	5/2018	Noda		A61B 6/54
2022/0249043	A1	*	8/2022	Liu		B25J 9/047
2023/0091213	A1	*	3/2023	Haase		A61B 6/547
2023/0270501	A1	*	8/2023	Patel		A61B 6/102
						700/245

OTHER PUBLICATIONS

“BusinessWire: Corindus, A Siemens Healthineers Company” Found online at businesswire.com. Oct. 4, 2023. Reference dated Sep. 12, 2022. Retrieved from <https://www.businesswire.com/news/home/20220907006221/en/Corindus-A-Siemens-Healthineers-Company-Announces-Study-Results-Demonstrating-Safety-and-Effectiveness-of-CorPat>.*

“DAIC: Recently Introduced Angiography Imaging Technology.” Found online at dicardiology.com. Oct. 4, 2023. Reference dated Feb. 7, 2018. Retrieved from <https://www.dicardiology.com/article/recently-introduced-angiography-imaging-technology>.*

“MedImaging: Canon Medical Systems Showcases Wide Product Lineup in Vienna.” Found online at medimaging.net. Oct. 4, 2023. Reference dated Feb. 28, 2019. Retrieved from <https://www.medimaging.net/ecr-2019/articles/294777078/canon-medical-systems-showcases-wide-product-lineup-in-vienna.html>.*

* cited by examiner

FIG. 1

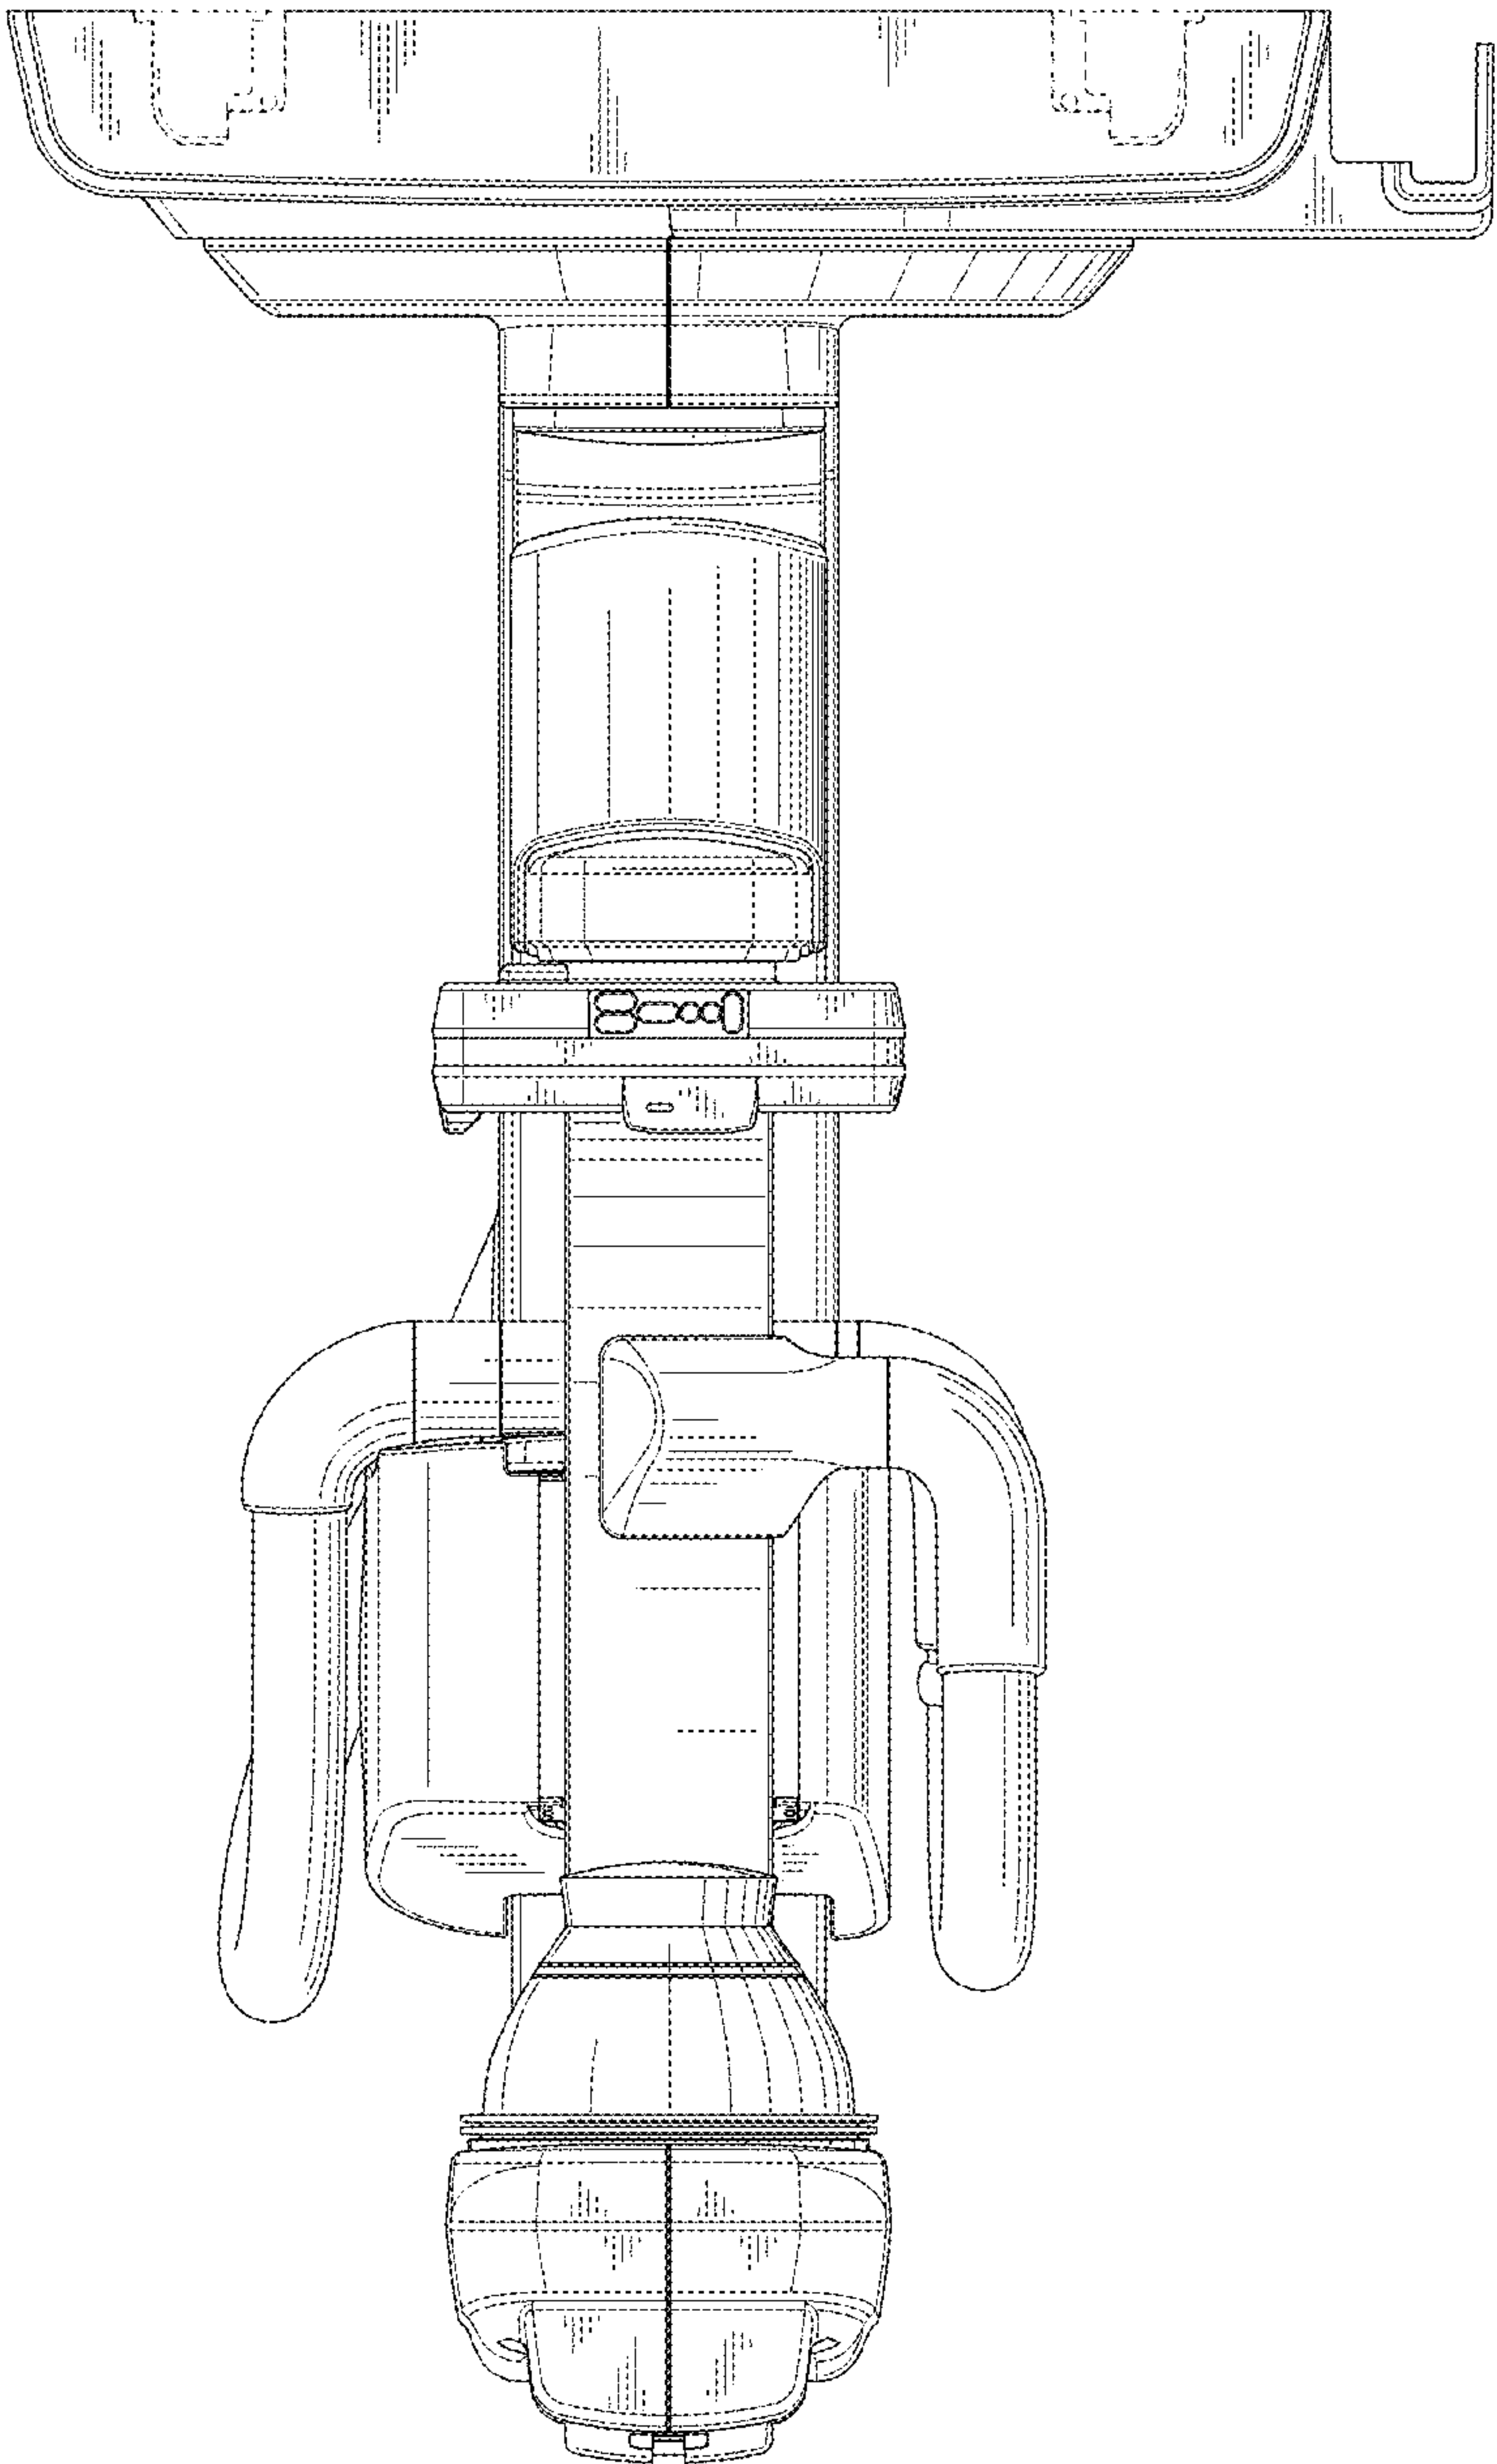


FIG. 2

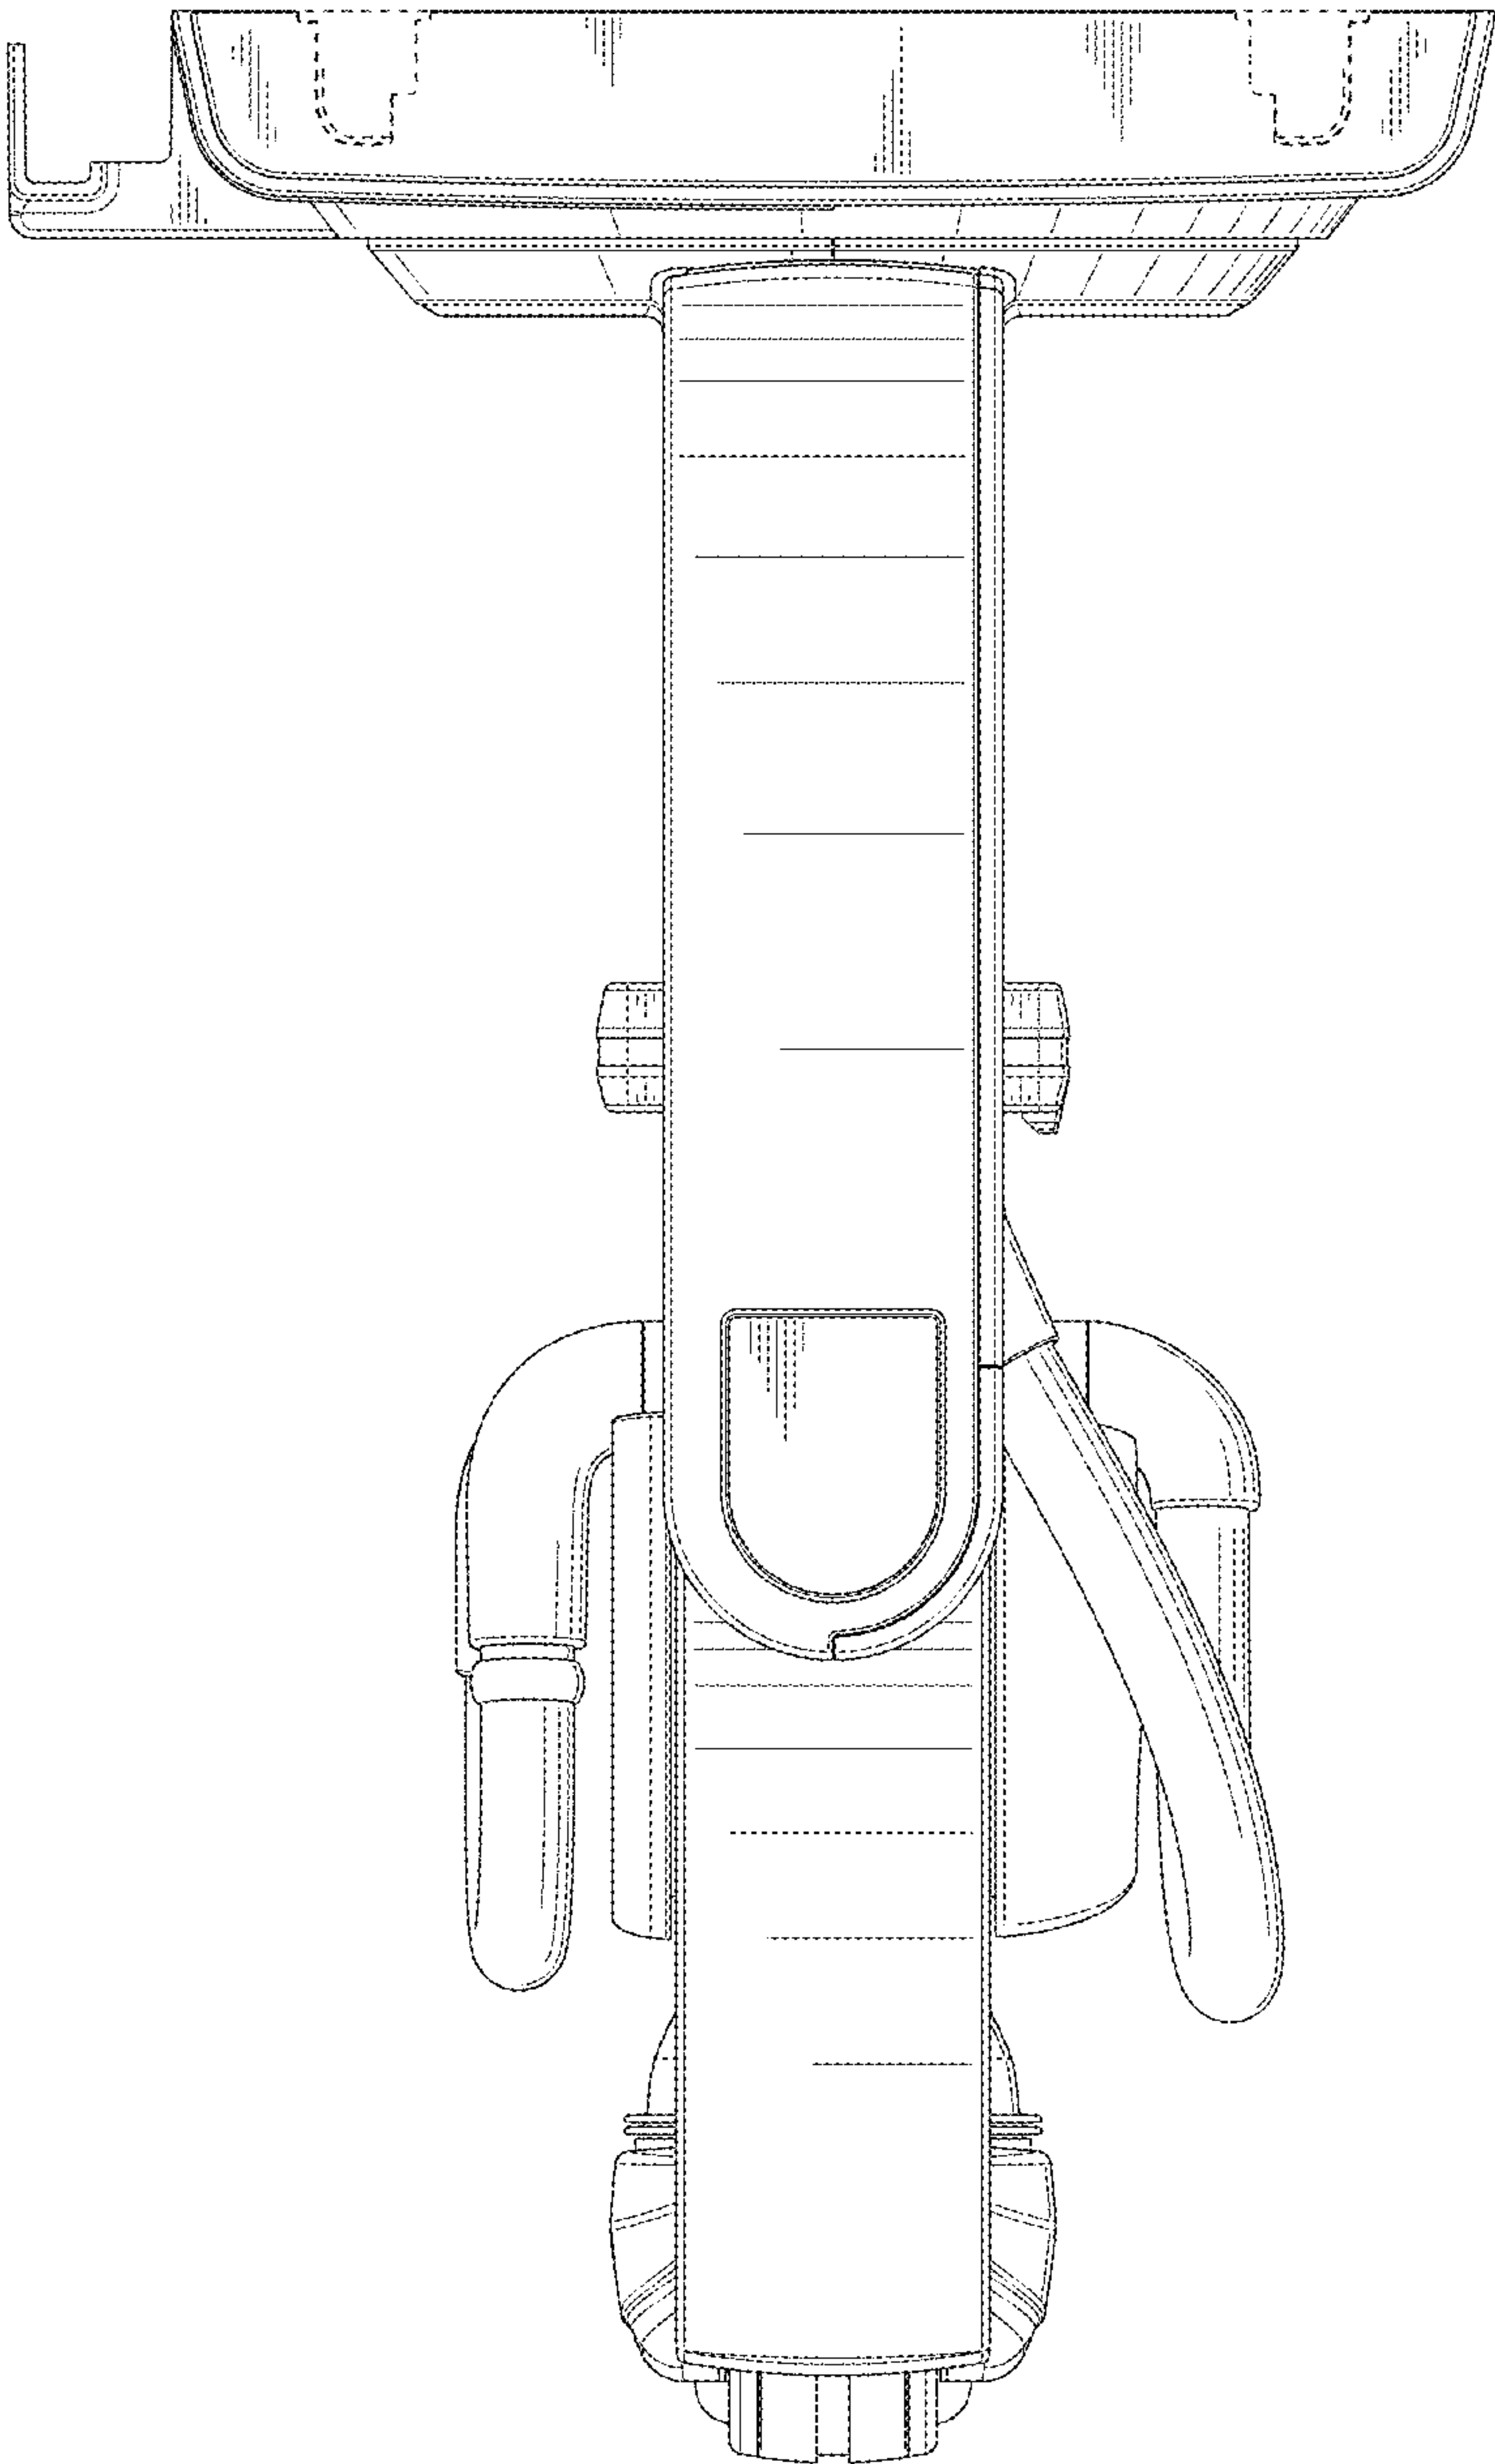


FIG. 3

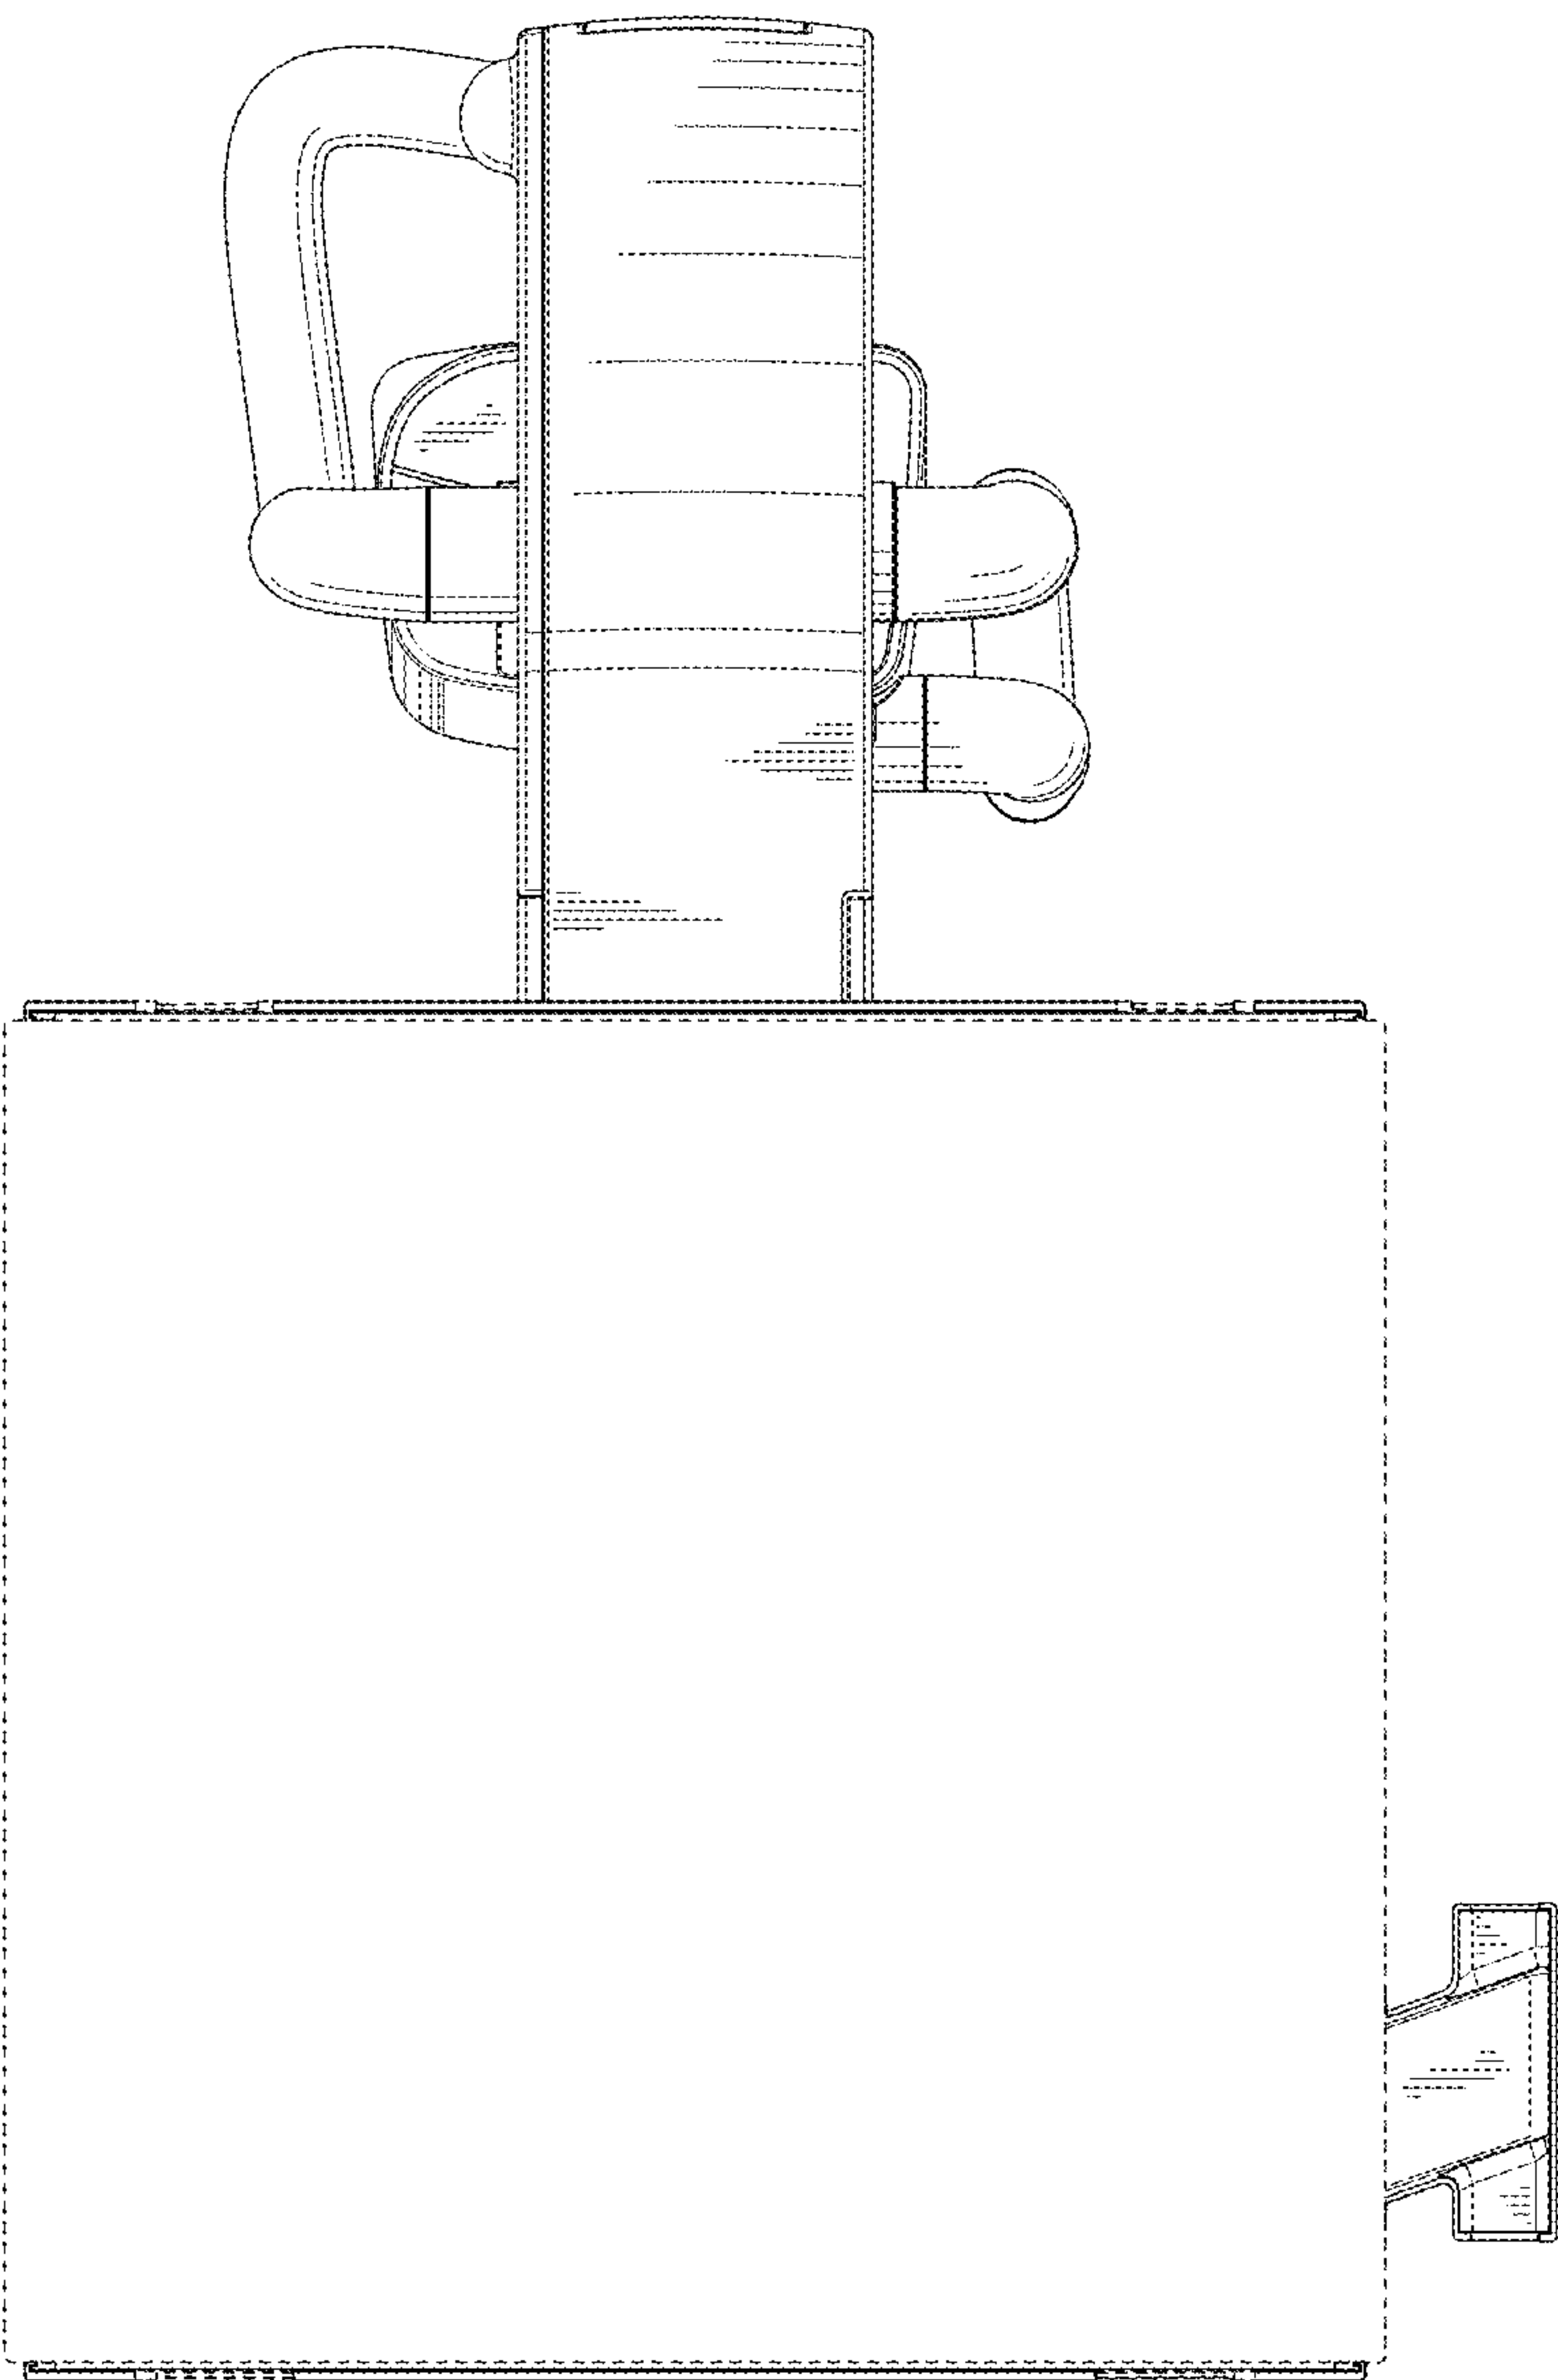


FIG. 4

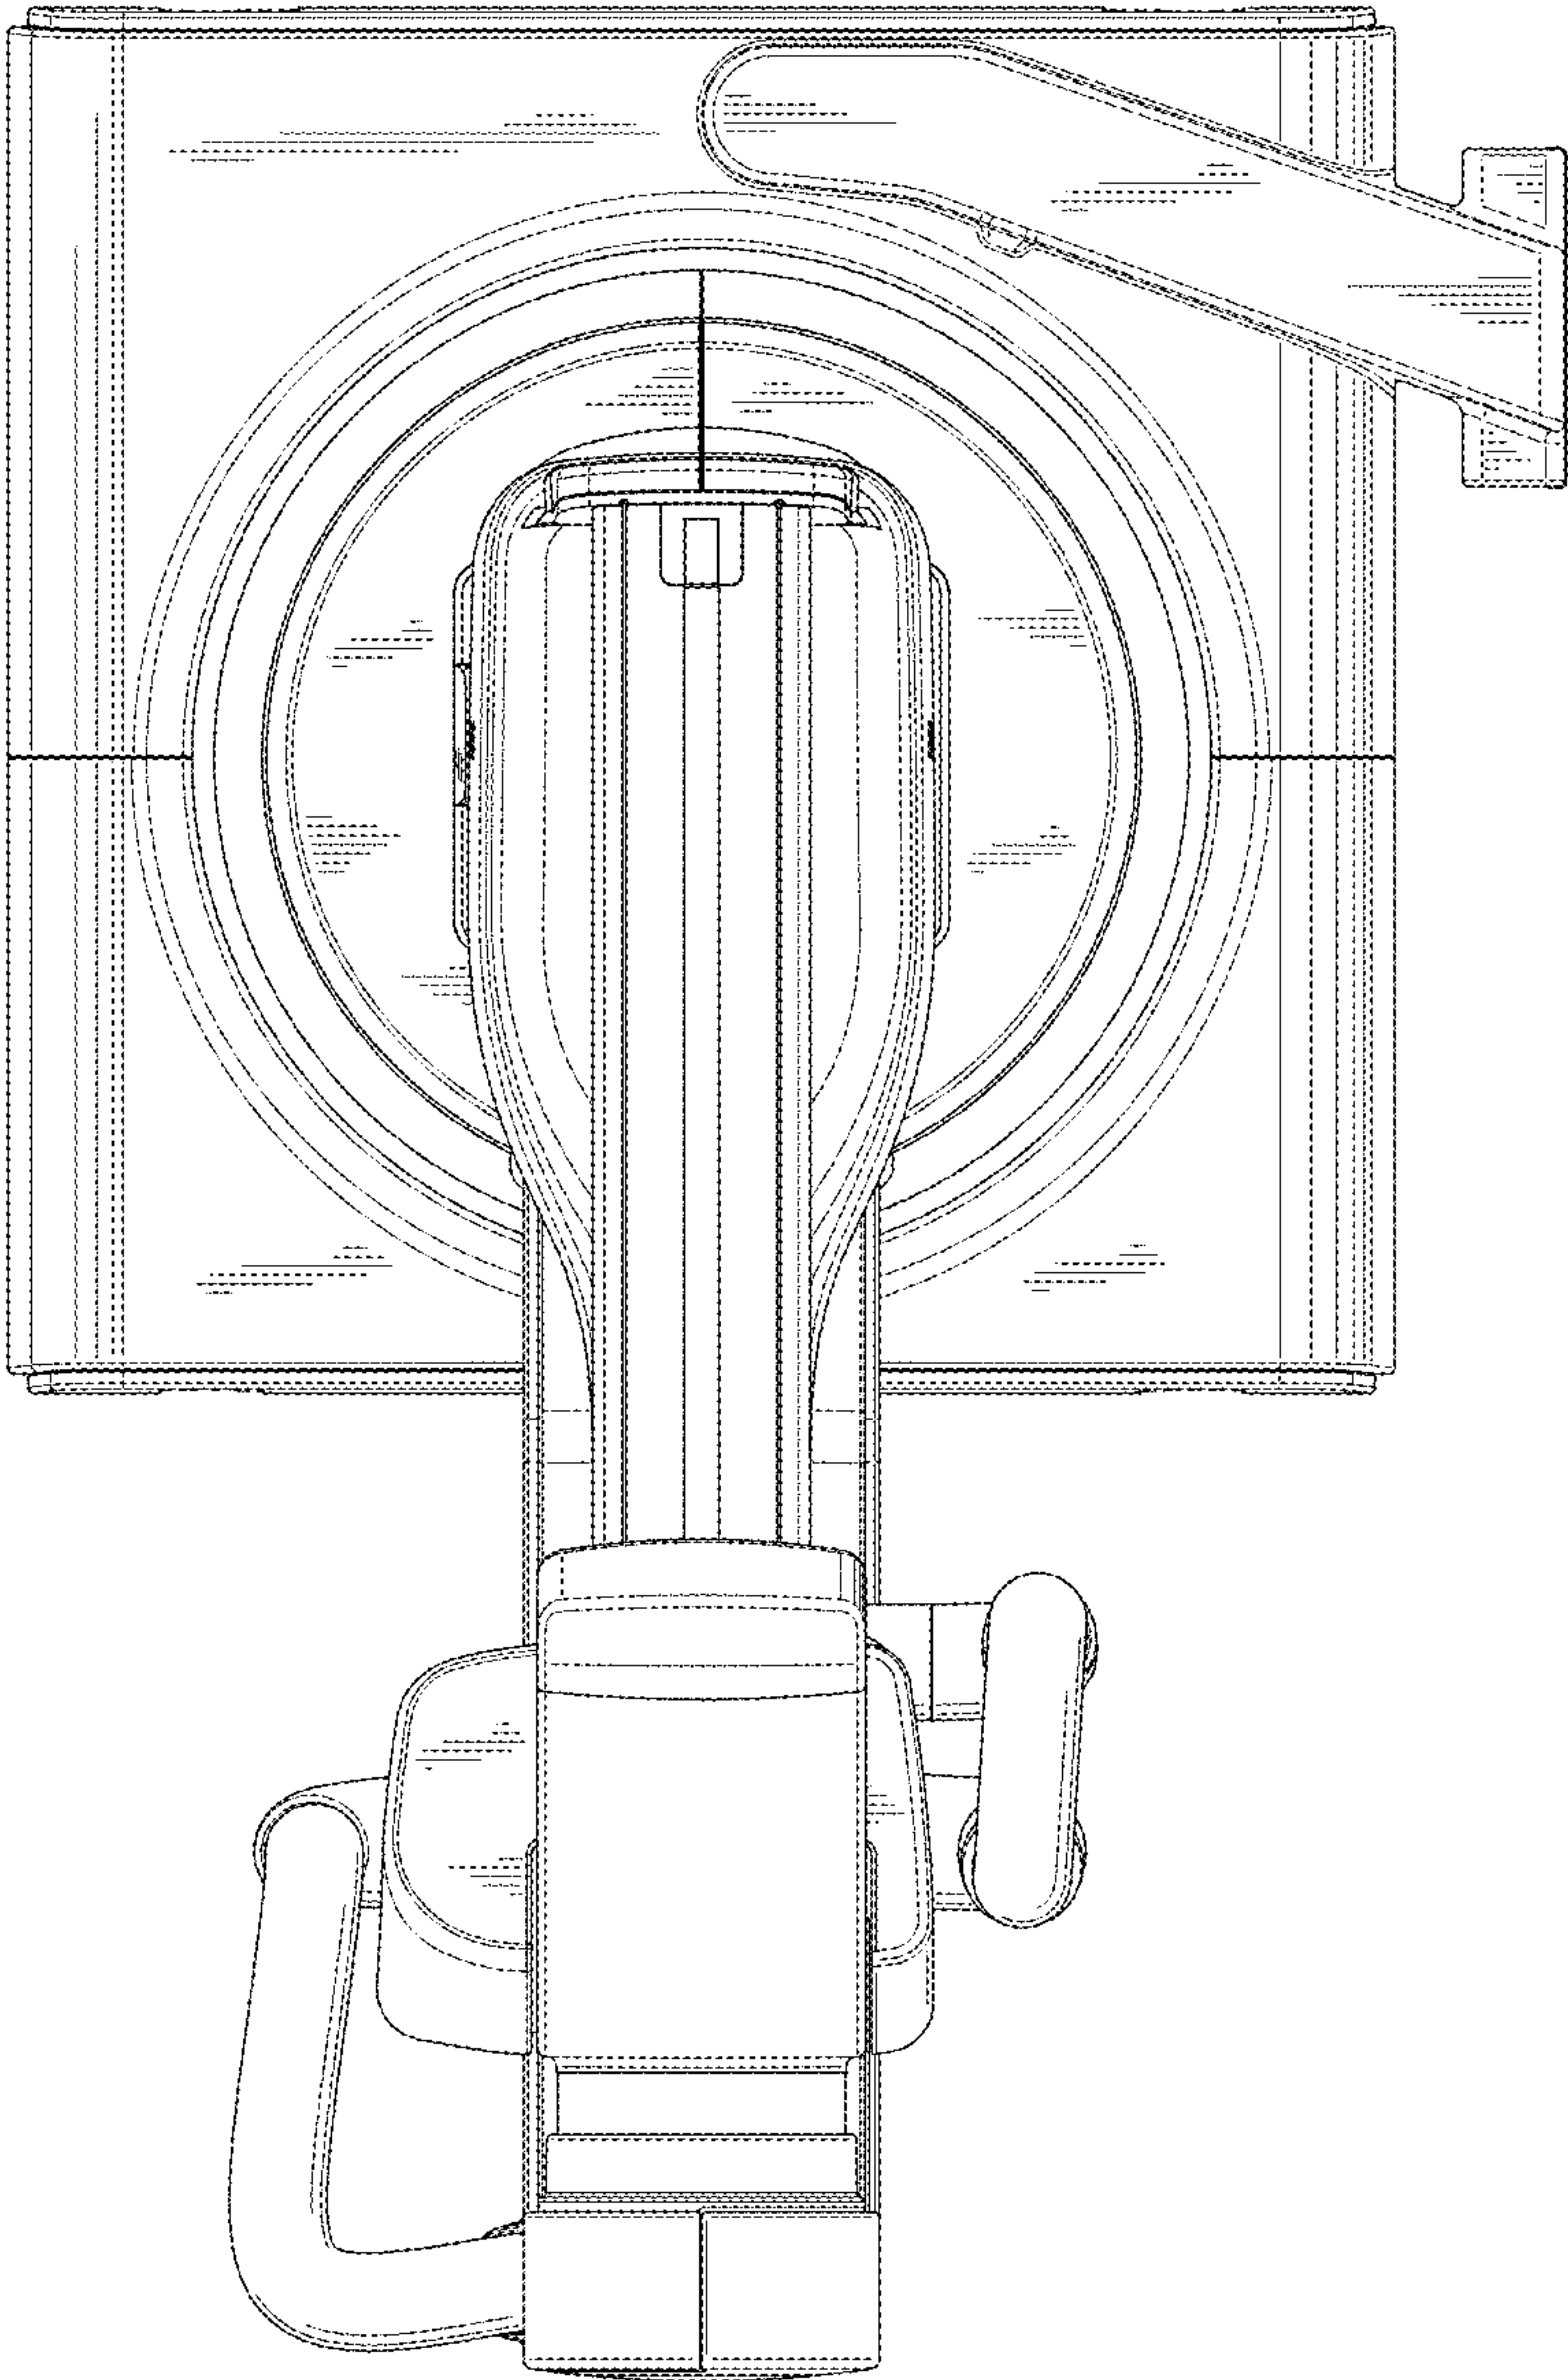


FIG. 5

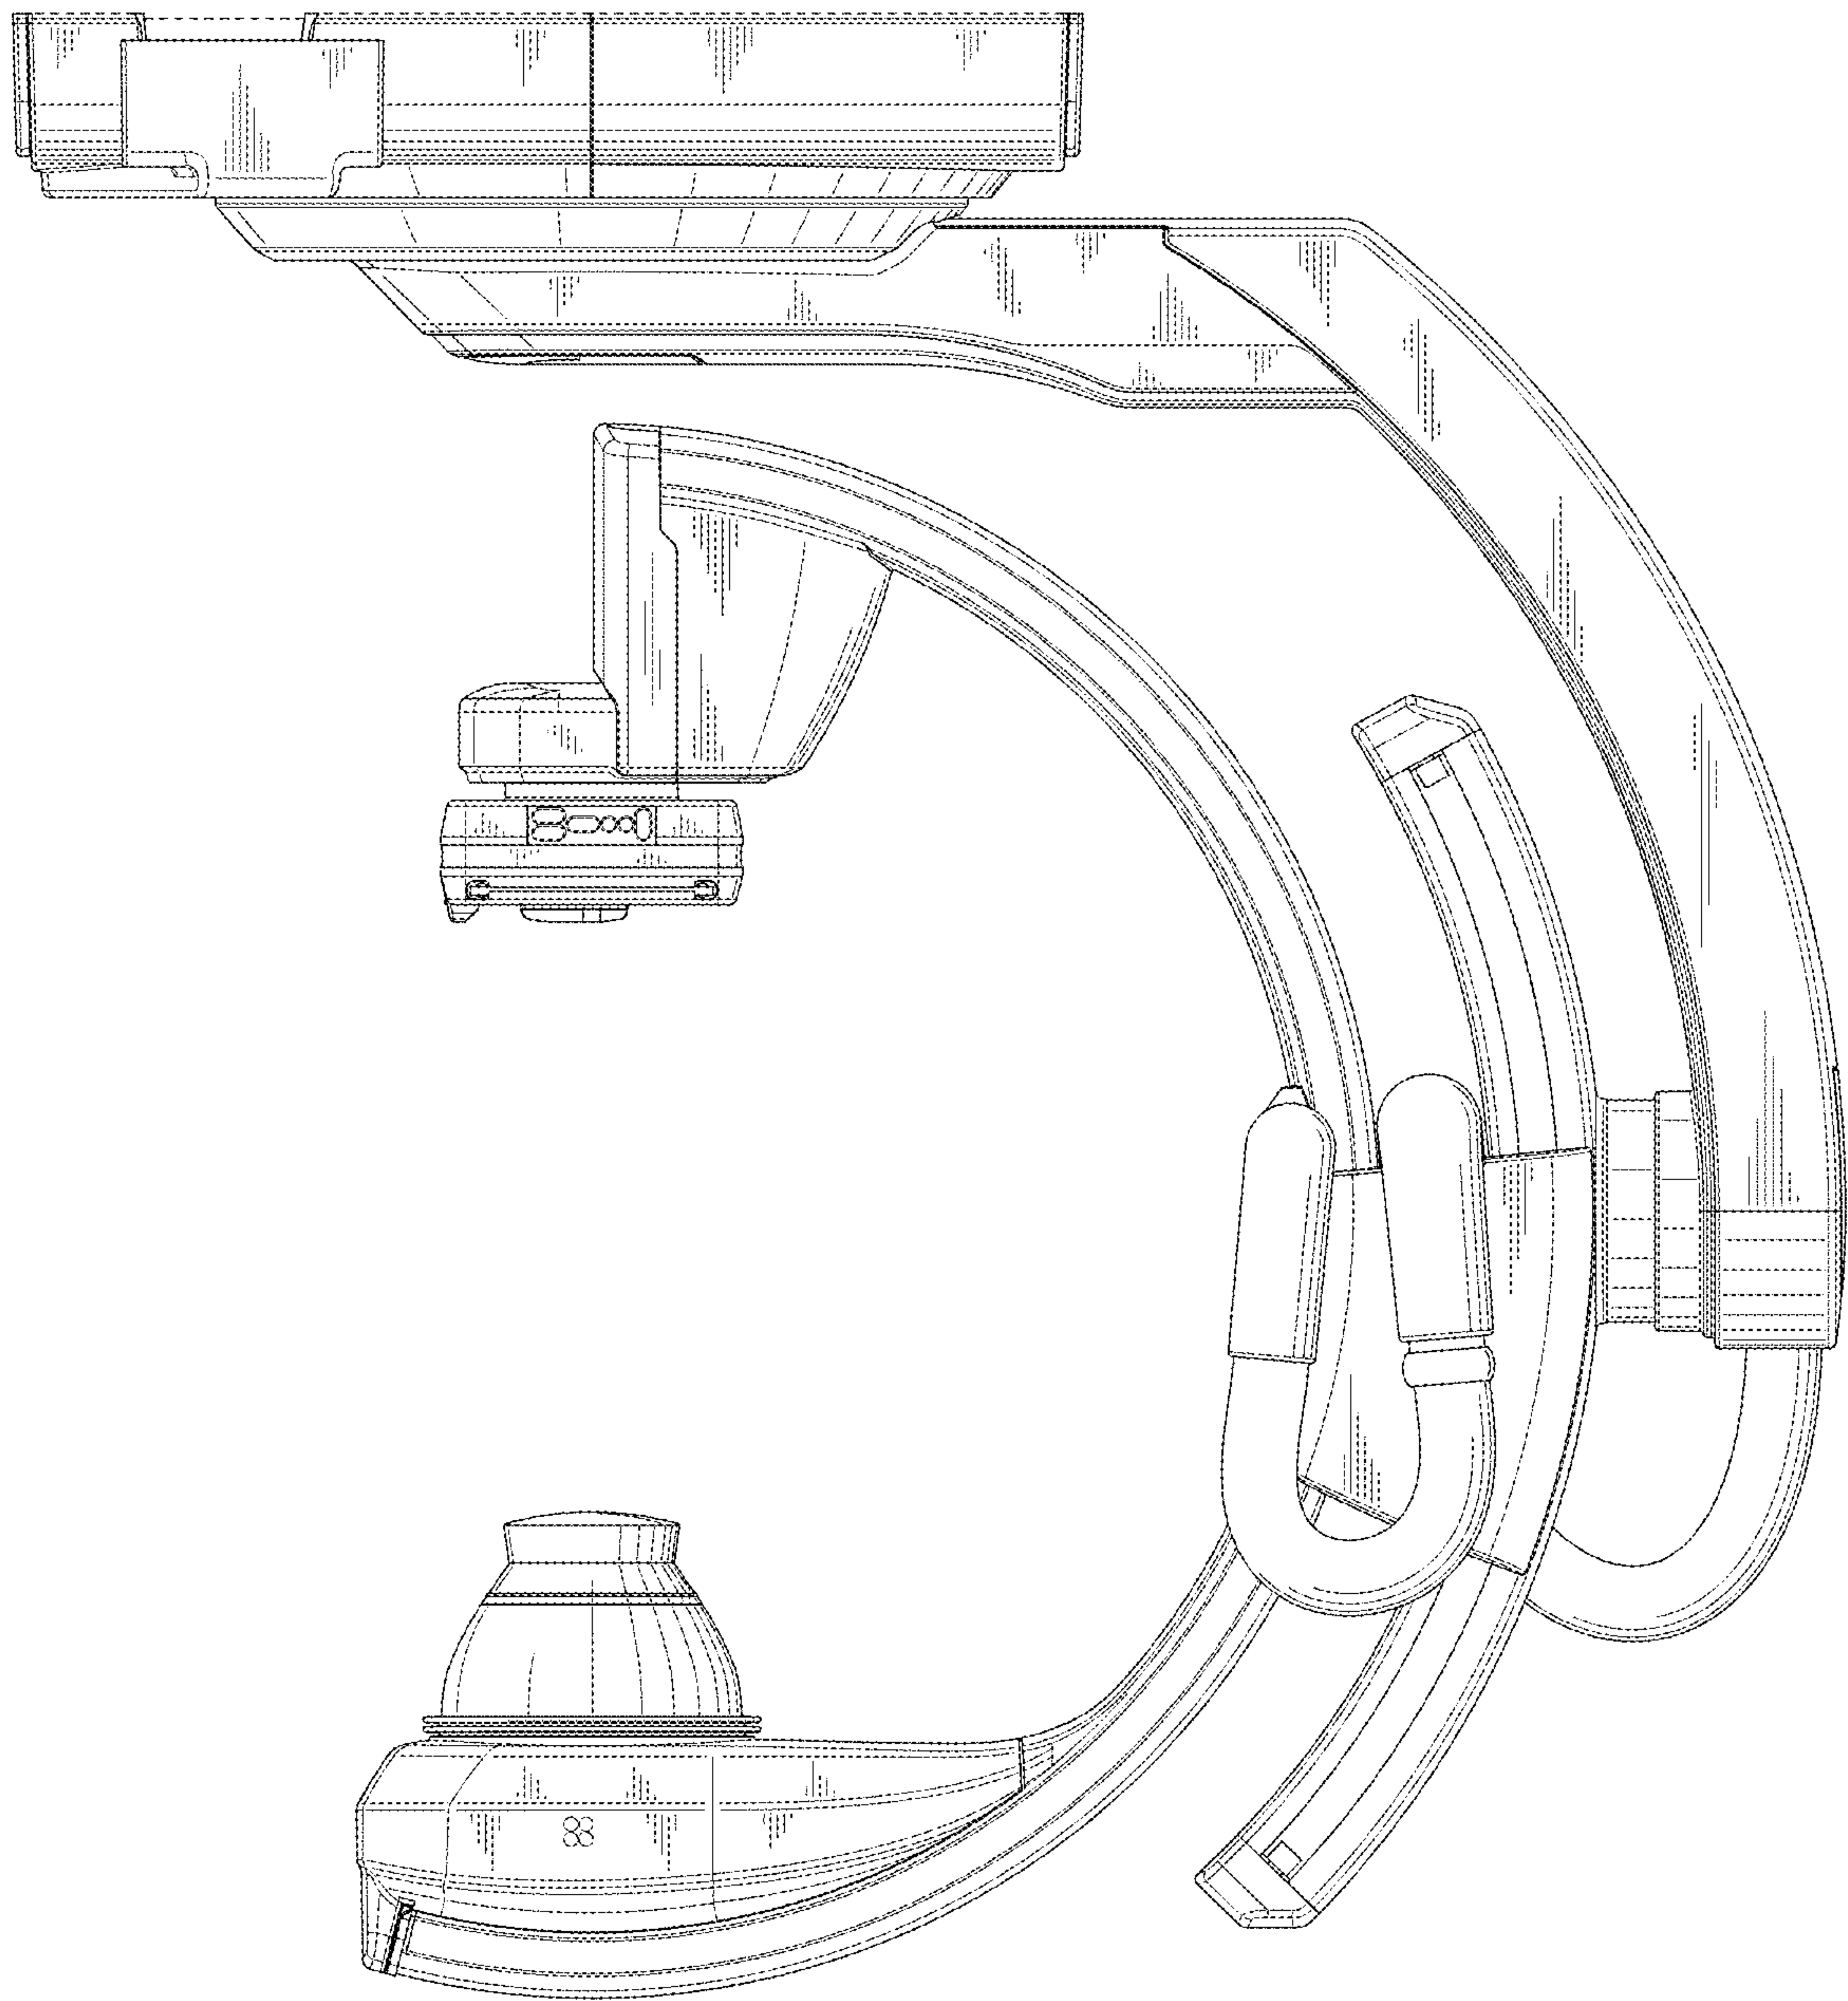


FIG. 6

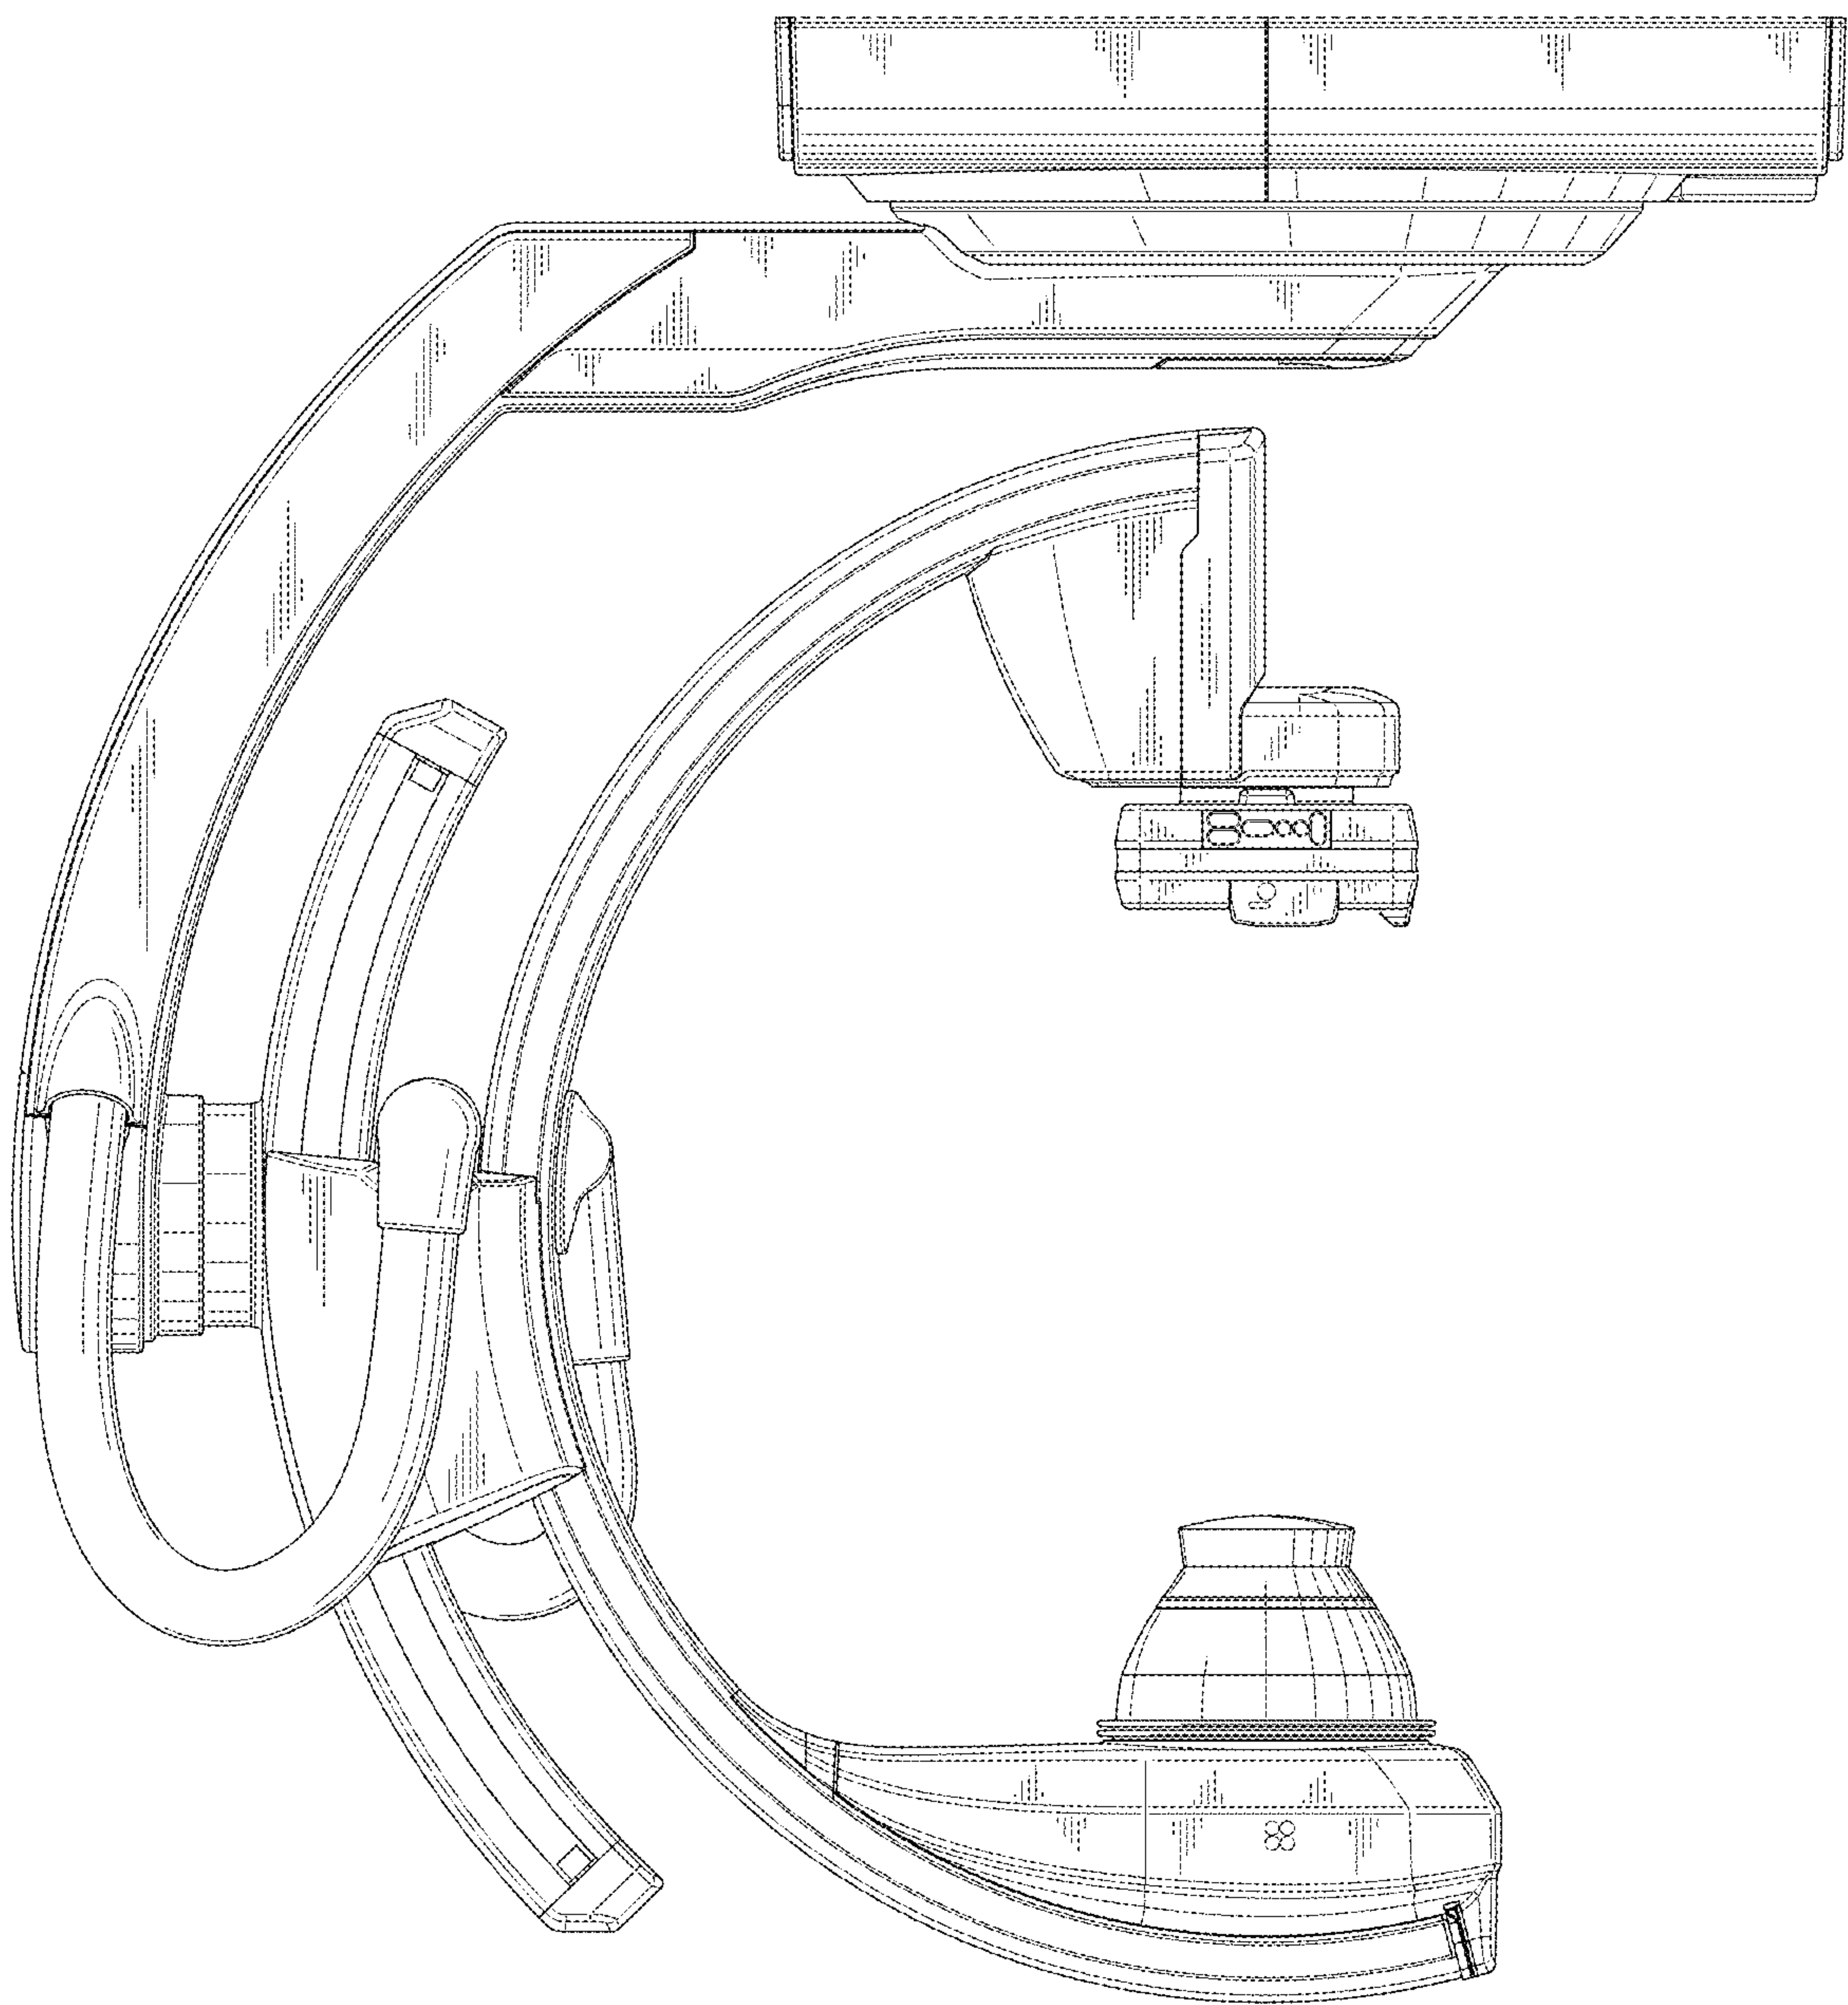


FIG. 7

